

 **ANALYTICAL REPORT****PREPARED FOR**

Attn: Terri Choy
AECOM

1001 Bishop Street
Honolulu HI 96813

Generated 3/9/2023 3:41 PM

JOB DESCRIPTION

Red Hill - AFFF Assessment Sampling

JOB NUMBER

580-124266-1

Eurofins Seattle

Job Notes

This report is issued solely for the use of the person or company to whom it is addressed. Any use, copying or disclosure other than by the intended recipient is unauthorized. If you have received this report in error, please notify the sender and destroy this report immediately. This report shall not be reproduced except in full, without prior express written approval by the laboratory.

The data in the report relate to the field sample(s) as received by the laboratory and associated QC. All results have been reviewed and have been found to be compliant with laboratory and accreditation requirements, with the exception of the noted deviation(s). For questions, please contact the Project Manager.

The test results in this report relate only to the samples as received by the laboratory and will meet all requirements of the methodology, with any exceptions noted. This report shall not be reproduced except in full, without the express written approval of the laboratory. All questions should be directed to the Eurofins Environment Testing Northwest, LLC Project Manager.

Authorization



Generated
3/9/2023 3:41 PM

Authorized for release by
Marie E Walker, Senior Project Manager
M.Elaine.Walker@et.eurofinsus.com
253 248-4972

Table of Contents

Cover Title Page	1
Data Summaries	5
Definitions	5
Case Narrative	6
Detection Summary	7
Client Sample Results	8
Default Detection Limits	9
QC Sample Results	10
QC Association	11
Chronicle	12
Certification Summary	13
Method Summary	14
Sample Summary	15
Manual Integration Summary	16
Reagent Traceability	19
COAs	20
Organic Sample Data	32
GC Semi VOA	32
Method 8015C - DAI Glycols	32
Method 8015C - DAI Glycols QC Summary	33
Method 8015C - DAI Glycols Sample Data	39
Standards Data	45
Method 8015C - DAI Glycols ICAL Data	45
Method 8015C - DAI Glycols CCAL Data	89
Raw QC Data	106
Method 8015C - DAI Glycols Blank Data	106

Table of Contents

Method 8015C - DAI Glycols LCS/LCSD Data	109
Method 8015C - DAI Glycols MS/MSD Data	117
Method 8015C - DAI Glycols Run Logs	125
Method 8015C - DAI Glycols Prep Data	126
Subcontracted Data	127
Shipping and Receiving Documents	128
Client Chain of Custody	129
Sample Receipt Checklist	133

Definitions/Glossary

Client: AECOM
Project/Site: Red Hill - AFFF Assessment Sampling

Job ID: 580-124266-1

Qualifiers

GC Semi VOA

Qualifier	Qualifier Description
M	Manual integrated compound.
U	Undetected at the Limit of Detection.

Glossary

Abbreviation	These commonly used abbreviations may or may not be present in this report.
α	Listed under the "D" column to designate that the result is reported on a dry weight basis
%R	Percent Recovery
CFL	Contains Free Liquid
CFU	Colony Forming Unit
CNF	Contains No Free Liquid
DER	Duplicate Error Ratio (normalized absolute difference)
Dil Fac	Dilution Factor
DL	Detection Limit (DoD/DOE)
DL, RA, RE, IN	Indicates a Dilution, Re-analysis, Re-extraction, or additional Initial metals/anion analysis of the sample
DLC	Decision Level Concentration (Radiochemistry)
EDL	Estimated Detection Limit (Dioxin)
LOD	Limit of Detection (DoD/DOE)
LOQ	Limit of Quantitation (DoD/DOE)
MCL	EPA recommended "Maximum Contaminant Level"
MDA	Minimum Detectable Activity (Radiochemistry)
MDC	Minimum Detectable Concentration (Radiochemistry)
MDL	Method Detection Limit
ML	Minimum Level (Dioxin)
MPN	Most Probable Number
MQL	Method Quantitation Limit
NC	Not Calculated
ND	Not Detected at the reporting limit (or MDL or EDL if shown)
NEG	Negative / Absent
POS	Positive / Present
PQL	Practical Quantitation Limit
PRES	Presumptive
QC	Quality Control
RER	Relative Error Ratio (Radiochemistry)
RL	Reporting Limit or Requested Limit (Radiochemistry)
RPD	Relative Percent Difference, a measure of the relative difference between two points
TEF	Toxicity Equivalent Factor (Dioxin)
TEQ	Toxicity Equivalent Quotient (Dioxin)
TNTC	Too Numerous To Count

CASE NARRATIVE
Client: AECOM
Project: Red Hill - AFFF Assessment Sampling
Report Number: 580-124266-1

This case narrative is in the form of an exception report, where only the anomalies related to this report, method specific performance and/or QA/QC issues are discussed. If there are no issues to report, this narrative will include a statement that documents that there are no relevant data issues.

It should be noted that samples with elevated Reporting Limits (RLs) resulting from a dilution may not be able to satisfy customer reporting limits in some cases. Such increases in the RLs are an unavoidable but acceptable consequence of sample dilution that enables quantification of target analytes within the calibration range of the instrument or that reduces the interferences thereby enabling the quantification of target analytes.

Calculations are performed before rounding to avoid round-off errors in calculated results.

All holding times were met and proper preservation noted for the methods performed on these samples, unless otherwise detailed in the individual sections below.

RECEIPT

Two samples were received on 3/4/2023 9:00 AM. Unless otherwise noted below, the samples arrived in good condition, and where required, properly preserved and on ice. The temperature of the cooler at receipt was 5.9° C.

Note: All samples which require thermal preservation are considered acceptable if the arrival temperature is within 2C of the required temperature or method specified range. For samples with a specified temperature of 4C, samples with a temperature ranging from just above freezing temperature of water to 6C shall be acceptable. Samples that are hand delivered immediately following collection may not meet these criteria, however they will be deemed acceptable according to NELAC standards, if there is evidence that the chilling process has begun, such as arrival on ice, etc.

GLYCOLS

Samples AF-RHMW03-WGN01LF-2302W4 (580-124266-1) and AF-RHMW02-WGN01LF-2302W4 (580-124266-2) were analyzed for glycols in accordance with EPA SW-846 Method 8015B - DAI. The samples were analyzed on 03/08/2023.

No analytical or quality issues were noted, other than those described above or in the Definitions/Glossary page.

Detection Summary

Client: AECOM
Project/Site: Red Hill - AFFF Assessment Sampling

Job ID: 580-124266-1

Client Sample ID: AF-RHMW03-WGN01LF-2302W4

Lab Sample ID: 580-124266-1

No Detections.

Client Sample ID: AF-RHMW02-WGN01LF-2302W4

Lab Sample ID: 580-124266-2

No Detections.

This Detection Summary does not include radiochemical test results.

Client Sample Results

Client: AECOM
Project/Site: Red Hill - AFFF Assessment Sampling

Job ID: 580-124266-1

Client Sample ID: AF-RHMW03-WGN01LF-2302W4

Lab Sample ID: 580-124266-1

Date Collected: 03/02/23 12:45

Matrix: Water

Date Received: 03/04/23 09:00

Method: SW846 8015C GLY - Glycols- Direct Injection (GC/FID)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
2-(2-Butoxyethoxy)ethanol	3.0	U M	5.0	1.1	mg/L			03/08/23 05:18	1

Client Sample ID: AF-RHMW02-WGN01LF-2302W4

Lab Sample ID: 580-124266-2

Date Collected: 03/02/23 11:10

Matrix: Water

Date Received: 03/04/23 09:00

Method: SW846 8015C GLY - Glycols- Direct Injection (GC/FID)

Analyte	Result	Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
2-(2-Butoxyethoxy)ethanol	3.0	U M	5.0	1.1	mg/L			03/08/23 05:42	1

Default Detection Limits

Client: AECOM

Job ID: 580-124266-1

Project/Site: Red Hill - AFFF Assessment Sampling

Method: 8015C GLY - Glycols- Direct Injection (GC/FID)

Analyte	LOQ	DL	Units
2-(2-Butoxyethoxy)ethanol	5.0	1.1	mg/L

QC Sample Results

Client: AECOM
 Project/Site: Red Hill - AFFF Assessment Sampling

Job ID: 580-124266-1

Method: 8015C GLY - Glycols- Direct Injection (GC/FID)

Lab Sample ID: MB 680-766428/17
Matrix: Water
Analysis Batch: 766428

Client Sample ID: Method Blank
Prep Type: Total/NA

Analyte	MB Result	MB Qualifier	LOQ	DL	Unit	D	Prepared	Analyzed	Dil Fac
2-(2-Butoxyethoxy)ethanol	3.0	U M	5.0	1.1	mg/L			03/07/23 22:18	1

Lab Sample ID: LCS 680-766428/13
Matrix: Water
Analysis Batch: 766428

Client Sample ID: Lab Control Sample
Prep Type: Total/NA

Analyte	Spike Added	LCS Result	LCS Qualifier	Unit	D	%Rec	%Rec Limits
2-(2-Butoxyethoxy)ethanol	20.0	21.5		mg/L		107	50 - 150

Lab Sample ID: LCSD 680-766428/14
Matrix: Water
Analysis Batch: 766428

Client Sample ID: Lab Control Sample Dup
Prep Type: Total/NA

Analyte	Spike Added	LCSD Result	LCSD Qualifier	Unit	D	%Rec	%Rec Limits	RPD	RPD Limit
2-(2-Butoxyethoxy)ethanol	20.0	23.1		mg/L		116	50 - 150	7	50

Lab Sample ID: 580-124266-2 MS
Matrix: Water
Analysis Batch: 766428

Client Sample ID: AF-RHMW02-WGN01LF-2302W4
Prep Type: Total/NA

Analyte	Sample Result	Sample Qualifier	Spike Added	MS Result	MS Qualifier	Unit	D	%Rec	%Rec Limits
2-(2-Butoxyethoxy)ethanol	3.0	U M	20.0	26.0		mg/L		130	50 - 150

Lab Sample ID: 580-124266-2 MSD
Matrix: Water
Analysis Batch: 766428

Client Sample ID: AF-RHMW02-WGN01LF-2302W4
Prep Type: Total/NA

Analyte	Sample Result	Sample Qualifier	Spike Added	MSD Result	MSD Qualifier	Unit	D	%Rec	%Rec Limits	RPD	RPD Limit
2-(2-Butoxyethoxy)ethanol	3.0	U M	20.0	28.2		mg/L		141	50 - 150	8	50

QC Association Summary

Client: AECOM
Project/Site: Red Hill - AFFF Assessment Sampling

Job ID: 580-124266-1

GC Semi VOA

Analysis Batch: 766428

Lab Sample ID	Client Sample ID	Prep Type	Matrix	Method	Prep Batch
580-124266-1	AF-RHMMW03-WGN01LF-2302W4	Total/NA	Water	8015C GLY	
580-124266-2	AF-RHMMW02-WGN01LF-2302W4	Total/NA	Water	8015C GLY	
MB 680-766428/17	Method Blank	Total/NA	Water	8015C GLY	
LCS 680-766428/13	Lab Control Sample	Total/NA	Water	8015C GLY	
LCSD 680-766428/14	Lab Control Sample Dup	Total/NA	Water	8015C GLY	
580-124266-2 MS	AF-RHMMW02-WGN01LF-2302W4	Total/NA	Water	8015C GLY	
580-124266-2 MSD	AF-RHMMW02-WGN01LF-2302W4	Total/NA	Water	8015C GLY	

Lab Chronicle

Client: AECOM
Project/Site: Red Hill - AFFF Assessment Sampling

Job ID: 580-124266-1

Client Sample ID: AF-RHMW03-WGN01LF-2302W4

Lab Sample ID: 580-124266-1

Date Collected: 03/02/23 12:45

Matrix: Water

Date Received: 03/04/23 09:00

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Analyst	Lab	Prepared or Analyzed
Total/NA	Analysis	8015C GLY		1	766428	JCK	EET SAV	03/08/23 05:18

Client Sample ID: AF-RHMW02-WGN01LF-2302W4

Lab Sample ID: 580-124266-2

Date Collected: 03/02/23 11:10

Matrix: Water

Date Received: 03/04/23 09:00

Prep Type	Batch Type	Batch Method	Run	Dilution Factor	Batch Number	Analyst	Lab	Prepared or Analyzed
Total/NA	Analysis	8015C GLY		1	766428	JCK	EET SAV	03/08/23 05:42

Laboratory References:

EET SAV = Eurofins Savannah, 5102 LaRoche Avenue, Savannah, GA 31404, TEL (912)354-7858

Accreditation/Certification Summary

Client: AECOM
Project/Site: Red Hill - AFFF Assessment Sampling

Job ID: 580-124266-1

Laboratory: Eurofins Savannah

Unless otherwise noted, all analytes for this laboratory were covered under each accreditation/certification below.

Authority	Program	Identification Number	Expiration Date
ANAB	Dept. of Defense ELAP	L2463	09-22-24

The following analytes are included in this report, but the laboratory is not certified by the governing authority. This list may include analytes for which the agency does not offer certification.

Analysis Method	Prep Method	Matrix	Analyte
8015C GLY		Water	2-(2-Butoxyethoxy)ethanol

Method Summary

Client: AECOM

Job ID: 580-124266-1

Project/Site: Red Hill - AFFF Assessment Sampling

Method	Method Description	Protocol	Laboratory
8015C GLY	Glycols- Direct Injection (GC/FID)	SW846	EET SAV

Protocol References:

SW846 = "Test Methods For Evaluating Solid Waste, Physical/Chemical Methods", Third Edition, November 1986 And Its Updates.

Laboratory References:

EET SAV = Eurofins Savannah, 5102 LaRoche Avenue, Savannah, GA 31404, TEL (912)354-7858

Sample Summary

Client: AECOM

Job ID: 580-124266-1

Project/Site: Red Hill - AFFF Assessment Sampling

Lab Sample ID	Client Sample ID	Matrix	Collected	Received
580-124266-1	AF-RHMW03-WGN01LF-2302W4	Water	03/02/23 12:45	03/04/23 09:00
580-124266-2	AF-RHMW02-WGN01LF-2302W4	Water	03/02/23 11:10	03/04/23 09:00

GC SEMI VOA MANUAL INTEGRATION SUMMARY

Lab Name: Eurofins Savannah Job No.: 580-124266-1

SDG No.: _____

Instrument ID: CVGG2 Analysis Batch Number: 766428

Lab Sample ID: IC 680-766428/5 Client Sample ID: _____

Date Analyzed: 03/07/23 17:36 Lab File ID: GC07013.D GC Column: J&W DB WAX ID: 0.45 (mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Propylene glycol	6.35	Baseline Smoothing	SWK1	03/08/23 10:47
Ethylene glycol	6.53	Baseline Smoothing	SWK1	03/08/23 10:47

Lab Sample ID: IC 680-766428/6 Client Sample ID: _____

Date Analyzed: 03/07/23 18:00 Lab File ID: GC07014.D GC Column: J&W DB WAX ID: 0.45 (mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Propylene glycol	6.35	Baseline Smoothing	SWK1	03/08/23 10:48

Lab Sample ID: IC 680-766428/7 Client Sample ID: _____

Date Analyzed: 03/07/23 18:23 Lab File ID: GC07015.D GC Column: J&W DB WAX ID: 0.45 (mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Propylene glycol	6.36	Baseline Smoothing	SWK1	03/08/23 10:48

Lab Sample ID: ICIS 680-766428/8 Client Sample ID: _____

Date Analyzed: 03/07/23 18:46 Lab File ID: GC07016.D GC Column: J&W DB WAX ID: 0.45 (mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Propylene glycol	6.35	Baseline Smoothing	SWK1	03/08/23 10:48

Lab Sample ID: IC 680-766428/9 Client Sample ID: _____

Date Analyzed: 03/07/23 19:10 Lab File ID: GC07017.D GC Column: J&W DB WAX ID: 0.45 (mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Propylene glycol	6.36	Baseline Smoothing	SWK1	03/08/23 10:49
Ethylene glycol	6.54	Baseline Smoothing	SWK1	03/08/23 10:49

8015C GLY

GC SEMI VOA MANUAL INTEGRATION SUMMARY

Lab Name: Eurofins Savannah Job No.: 580-124266-1

SDG No.: _____

Instrument ID: CVGG2 Analysis Batch Number: 766428

Lab Sample ID: IC 680-766428/10 Client Sample ID: _____

Date Analyzed: 03/07/23 19:33 Lab File ID: GC07018.D GC Column: J&W DB WAX ID: 0.45 (mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Propylene glycol	6.37	Baseline Smoothing	SWK1	03/08/23 10:49
Ethylene glycol	6.54	Baseline Smoothing	SWK1	03/08/23 10:49

Lab Sample ID: IC 680-766428/11 Client Sample ID: _____

Date Analyzed: 03/07/23 19:57 Lab File ID: GC07019.D GC Column: J&W DB WAX ID: 0.45 (mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Propylene glycol	6.37	Baseline Smoothing	SWK1	03/08/23 10:49

Lab Sample ID: ICV 680-766428/12 CCV Client Sample ID: _____

Date Analyzed: 03/07/23 20:20 Lab File ID: GC07020.D GC Column: J&W DB WAX ID: 0.45 (mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
Propylene glycol	6.35	Baseline Smoothing	SWK1	03/08/23 10:50
Ethylene glycol	6.53	Baseline Smoothing	SWK1	03/08/23 10:50

Lab Sample ID: MB 680-766428/17 Client Sample ID: _____

Date Analyzed: 03/07/23 22:18 Lab File ID: GC07025.D GC Column: J&W DB WAX ID: 0.45 (mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
2-(2-Butoxyethoxy)ethanol		Invalid Compound ID	SWK1	03/08/23 11:13

Lab Sample ID: 580-124266-1 Client Sample ID: AF-RHMW03-WGN01LF-2302W4

Date Analyzed: 03/08/23 05:18 Lab File ID: GC07043.D GC Column: J&W DB WAX ID: 0.45 (mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
2-(2-Butoxyethoxy)ethanol		Invalid Compound ID	SWK1	03/08/23 11:20

8015C GLY

GC SEMI VOA MANUAL INTEGRATION SUMMARY

Lab Name: Eurofins Savannah Job No.: 580-124266-1

SDG No.: _____

Instrument ID: CVGG2 Analysis Batch Number: 766428

Lab Sample ID: 580-124266-2 Client Sample ID: AF-RHMW02-WGN01LF-2302W4

Date Analyzed: 03/08/23 05:42 Lab File ID: GC07044.D GC Column: J&W DB WAX ID: 0.45 (mm)

COMPOUND NAME	RETENTION TIME	MANUAL INTEGRATION		
		REASON	ANALYST	DATE
2-(2-Butoxyethoxy)ethanol		Invalid Compound ID	SWK1	03/08/23 11:20

REAGENT TRACEABILITY SUMMARY

Lab Name: Eurofins Savannah Job No.: 580-124266-1

SDG No.: _____

Reagent ID	Exp Date	Prep Date	Dilutant Used	Reagent Final Volume	Parent Reagent		Analyte	Concentration
					Reagent ID	Volume Added		
SG_Gly_CAL_00048	05/21/23		o2si, Lot 480919			(Purchased Reagent)	2,2'-Oxybisethanol	2000 ug/mL
							2-(2-Butoxyethoxy)ethanol	2000 ug/mL
							2-Butoxyethanol	2000 ug/mL
							4-Hydroxy-4-methyl-2-pentanone	2000 ug/mL
							Dipropylene Glycol Methyl Ether	2000 ug/mL
							Ethanol, 2-propoxy	2000 ug/mL
							Ethylene glycol	2000 ug/mL
							Propylene glycol	2000 ug/mL
SG_GLY_ISTD_00106	05/22/23		Agilent, Lot 0006720623			(Purchased Reagent)	n-Heptyl Alcohol	5000 ug/mL
SG_GlyICV_00055	08/21/23		o2si, Lot 454407			(Purchased Reagent)	2-(2-Butoxyethoxy)ethanol	2000 ug/mL

Reagent

SG_Gly_CAL_00048



ISO/IEC 17025 Accredited
Chemical Testing Lab
Cert. No. 3031.01



ISO 17034 Accredited
Reference Material Producer
Cert. No. 3031.02

Rev 0

Certificate of Analysis

Page 1 of 3

Catalog No.	Lot No.	Storage	Solvent	Date Received	Exp. Date
G34-120070-04	480919	≤ -10 °C	P/T Methanol		2-May-2024

Description:

ISO 17034 -Custom Volatiles Mix,105-12, 2000 & 4,000 mg/L, 1 mL

Container:

1 ml Ampule, Amber Glass

Certified Values:

The certified value is based on gravimetric and volumetric preparation of this Certified Reference Material (CRM). This CRM has been confirmed by GC/MS, GC, HPLC, UPLC/HRAM-MS, UV/VIS, Enzymatic, and/or wet chemistry techniques using internally developed method(s) against independent source(s). The uncertainty value is calculated for a 95% confidence interval with a *k* value of 2. The purity of neat materials not traceable to an ISO 17034:2016 accredited Reference Material Provider is traceable to internal analysis by GC, GC/MS, HPLC, Enzymatic, or wet chemistry techniques and compared to a National Metrological Institute such as NIST where feasible.

Compound	CAS No.	Purity (%)	Neat Material Lot No.	Concentration	
2-butoxyethanol	111-76-2	99.6	311.9.2P	1986 ± 100	mg/L
diethylene glycol butyl ether	112-34-5	99.8	2323.7.2P	2008 ± 100	mg/L
propyl cellosolve	2807-30-9	99.9	1570.7.2P	1980 ± 100	mg/L
dipropylene glycol monomethyl ether	34590-94-8	99.7	2333.7.2P	2014 ± 100	mg/L
ethylene glycol	107-21-1	100	307.201.1P	1968 ± 99	mg/L
di(ethylene glycol)	111-46-6	99.5	309.7.2P	1994 ± 100	mg/L
tri(ethylene glycol)	112-27-6	99.9	310.7.2.1.1P	1974 ± 110	mg/L
4-Hydroxy-4-methyl-2-pentanone	123-42-2	98	2334.286.1P	1991 ± 110	mg/L
1,2-propanediol	57-55-6	99.5	306.9.3P	1998 ± 100	mg/L
tetraethylene glycol	112-60-7	98	3754.7.1P	3959 ± 200	mg/L

Intended Uses:

This CRM is intended for use as a calibration standard or a quality control standard for chromatography equipment such as GC, GC/MS, HPLC, and HPLC/MS. It may also be used for various USEPA, NIOSH and ASTM methods.

Recommended storage container for ampuled products after opening is a 12 mm x 32 mm amber vial with screw cap Teflon lined silicon septum. The modeled % change per day can be calculated using the following:

Certificate of Analysis

Page 2 of 3

Catalog No. G34-120070-04

Lot No. 480919

Expiration Date 2 -May-2024

$$\% \text{ Change} = 116192x^{-2.578} + 40.383e^{-0.03y}$$

where x = boiling point of the most volatile analyte in the mix (in degrees K)

y = boiling point of the solvent (in degrees K)

This model assumes the container is stored at -10 °C and is unopened during storage. The user should determine what the acceptable error for their process is and calculate the maximum number of days the opened ampule should be stored.

Method of Preparation:

This standard was prepared gravimetrically using balances calibrated with National Institute of Standards and Technology (NIST) traceable weights (NIST Test Numbers 822/273070-06, 822/275141-07, 822/278993-10). Only calibrated Class A volumetric glassware and/or calibrated syringes were used to prepare this standard. Raw materials may have been checked for stoichiometry and purity prior to use. This standard has been analyzed against an independent source.

Packaging and Storage:

The solution should be stored according to the following storage requirements: ≤ -10 °C

Once the product is opened, it should be transferred to a vial with minimum head space if the product was received in a sealed ampule.

Glassware Calibration:

Only Class A glassware and/or calibrated syringes are used in the manufacture and quality control of standards. All glassware is calibrated using NIST traceable weights.

Weights and Balance Calibration:

Weights used to perform daily checks on balances are calibrated annually by the State of South Carolina Department of Agriculture Metrology Laboratory and are traceable to NIST. Balances are checked daily in accordance to procedure O2-LB-G-002. Balances are calibrated annually by an ISO/IEC 17025:2017 accredited metrology service.

Homogeneity:

Homogeneity has been established in accordance with internal procedure O2-QS-011 and has a maximum uncertainty of 0.1%. This is consistent with the intended use of this CRM. The homogeneity of this product has been confirmed by procedures consistent with ISO/IEC 17025:2017 and ISO 17034:2016. The homogeneity of this CRM is valid for sample sub-sizes that the end user can quantitatively reproduce.

Hazardous Information:

Refer to MSDS.

Calculation of Uncertainty:

The following equations are used to calculate the value of the expanded uncertainty:

$u = ku_c$ u = Expanded Uncertainty, k = the coverage factor at the 95% confidence level, k = 2, u_c = the combined uncertainty

$u_c = (u_{\text{char}}^2 + u_{\text{tran}}^2 + u_{\text{homo}}^2 + u_{\text{ls}}^2)^{1/2}$ where u_i are the individual uncertainty components for manufacturing, transportation, homogeneity, and shelf life. While no significant uncertainty was detected in the replicates, a minimum contribution to

Manufactured By:




Brian Stokes

3 -May-2022

Production Chemist I

Certified By:



Tyler Sherman

14 -Jun-2022

Quality Control Chemist I

Released By:



Susan Mathews

14 -Jun-2022

Quality Control Team Lead

7290B Investment Drive • North Charleston, SC 29418
Phone: 866.272.0932 • Fax: 866.509.5146 www.o2si.com

Certificate of Analysis

Catalog No. G34-120070-04

Lot No. 480919

Expiration Date 2 -May-2024

uncertainty was added for homogeneity and long term stability as described in ISO Guide 35:2017.


Expiration Information:

The stability of this product is based upon rigorous short term and long term testing of the solution for the certified value. These tests include the effect of temperature and packaging on the product. Studies on the short term instability have determined no contribution to instability as observed on the concentration under controlled transportation conditions. This standard is guaranteed until 2-May-2024

Quality Standard Documentation:

- ISO/IEC 17025:2017 "General Requirements for the Competence of Testing and Calibration" - Chemical Testing - Accredited A2LA Certificate Number 3031.01
- ISO 17034:2016 "General Requirements for the Competence of Reference Material Producers" - Reference Material Production - Accredited A2LA Certificate Number 3031.02

Manufactured By:



Brian Stokes

3 -May-2022

Production Chemist I

Certified By:



Tyler Sherman

14 -Jun-2022

Quality Control Chemist I

7290B Investment Drive • North Charleston, SC 29418
Phone: 866.272.0932 • Fax: 866.509.5146 www.o2si.com

Released By:



Susan Mathews

14 -Jun-2022

Quality Control Team Lead

Reagent

SG_GLY_ISTD_00106

Reference Material Certificate
Product Information Sheet

Product Name: Custom Standard

Lot Number: 0006720623

Product Number: CUS-6046

Lot Issue Date: 15-Dec-2022

Storage Conditions: Store at Room Temperature (15° to 30°C).

Expiration Date: 31-Jan-2025

Component Name	CERTIFIED VALUES		CAS#	Analyte Lot
	Concentration	Expanded Uncertainty		
n-heptanol	5001	± 25 µg/mL	000111-70-6	RM04540

Matrix: methanol (methyl alcohol)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCCL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Expiration of Certification:


The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.



Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:


Monica Bourgeois
QMS Representative



RM was produced in accordance with the TUV/SUD registered ISO 9001:2015 Quality Management System. Cert# 951215321

Page: 2 of 2

www.agilent.com/quality/
CSD-QA-015.1

ISO 17025

ISO 17034 Cert
No. AR-1936

Reagent

SG_GlyICV_00055



ISO/IEC 17025 Accredited
Chemical Testing Lab
Cert. No. 3031.01



ISO 17034 Accredited
Reference Material Producer
Cert. No. 3031.02

Rev 0

Certificate of Analysis

Page 1 of 3

Catalog No.	Lot No.	Storage	Solvent	Date Received	Exp. Date
G34-120070-04-SS	454407	≤ -10 °C	P/T Methanol		1-Jul-2023

Description:

ISO 17034 -Custom Volatiles Mix, 105-12, Second Source, 2000 & 4,000 mg/L, 1 mL

Container:

1 ml Ampule, Amber Glass

Certified Values:

The certified value is based on gravimetric and volumetric preparation of this Certified Reference Material (CRM). This CRM has been confirmed by GC/MS, GC, HPLC, UPLC/HRAM-MS, UV/VIS, Enzymatic, and/or wet chemistry techniques using internally developed method(s) against independent source(s). The uncertainty value is calculated for a 95% confidence interval with a *k* value of 2. The purity of neat materials not traceable to an ISO 17034:2016 accredited Reference Material Provider is traceable to internal analysis by GC, GC/MS, HPLC, Enzymatic, or wet chemistry techniques and compared to a National Metrological Institute such as NIST where feasible.

Compound	CAS No.	Purity (%)	Neat Material Lot No.	Concentration
2-butoxyethanol	111-76-2	99.5	311.7.1.1S	1994 ± 100 mg/L
diethylene glycol butyl ether	112-34-5	99.8	2323.7.2.1S	1992 ± 100 mg/L
2-propoxyethanol	2807-30-9	99.5	1570.7.1S	1998 ± 110 mg/L
dipropylene glycol monomethyl ether	34590-94-8	99.7	2333.7.2.1S	1998 ± 100 mg/L
ethylene glycol	107-21-1	100	307.201.1.1S	2016 ± 100 mg/L
di(ethylene glycol)	111-46-6	99.9	309.7.1.1S	1998 ± 100 mg/L
tri(ethylene glycol)	112-27-6	99.9	310.7.3.1S	2010 ± 100 mg/L
4-Hydroxy-4-methyl-2-pentanone	123-42-2	98	2334.286.1.1S	2003 ± 110 mg/L
1,2-propanediol	57-55-6	99.6	306.370.1.1S	2004 ± 110 mg/L
tetraethylene glycol	112-60-7	98	3754.7.1.1S	4049 ± 200 mg/L

Intended Uses:

This CRM is intended for use as a calibration standard or a quality control standard for chromatography equipment such as GC, GC/MS, HPLC, and HPLC/MS. It may also be used for various USEPA, NIOSH and ASTM methods.

Recommended storage container for ampuled products after opening is a 12 mm x 32 mm amber vial with screw cap Teflon lined silicon septum. The modeled % change per day can be calculated using the following:

Certificate of Analysis

Page 2 of 2

Catalog No. G34-120070-04-SS

Lot No. 454407

Expiration Date 1 -Jul-2023

$$\% \text{ Change} = 116192x^{-2.578} + 40.383e^{-0.03y}$$

where x = boiling point of the most volatile analyte in the mix (in degrees K)
y = boiling point of the solvent (in degrees K)

This model assumes the container is stored at -10 °C and is unopened during storage. The user should determine what the acceptable error for their process is and calculate the maximum number of days the opened ampule should be stored.

Method of Preparation:

This standard was prepared gravimetrically using balances calibrated with National Institute of Standards and Technology (NIST) traceable weights (NIST Test Numbers 822/273070-06, 822/275141-07, 822/278993-10). Only calibrated Class A volumetric glassware and/or calibrated syringes were used to prepare this standard. Raw materials may have been checked for stoichiometry and purity prior to use. This standard has been analyzed against an independent source.

Packaging and Storage:

The solution should be stored according to the following storage requirements: ≤ -10 °C

Once the product is opened, it should be transferred to a vial with minimum head space if the product was received in a sealed ampule.

Glassware Calibration:

Only Class A glassware and/or calibrated syringes are used in the manufacture and quality control of standards. All glassware is calibrated using NIST traceable weights.

Weights and Balance Calibration:

Weights used to perform daily checks on balances are calibrated annually by the State of South Carolina Department of Agriculture Metrology Laboratory and are traceable to NIST. Balances are checked daily in accordance to procedure O2-LB-G-002. Balances are calibrated annually by an ISO/IEC 17025:2017 accredited metrology service.

Homogeneity:

Homogeneity has been established in accordance with internal procedure O2-QS-011 and has a maximum uncertainty of 0.1%. This is consistent with the intended use of this CRM. The homogeneity of this product has been confirmed by procedures consistent with ISO/IEC 17025:2017 and ISO 17034:2016. The homogeneity of this CRM is valid for sample sub-sizes that the end user can quantitatively reproduce.

Hazardous Information:

Refer to MSDS.

Calculation of Uncertainty:

The following equations are used to calculate the value of the expanded uncertainty:

$u = ku_c$ u = Expanded Uncertainty, k = the coverage factor at the 95% confidence level, k = 2, u_c = the combined uncertainty

$u_c = (u_{\text{char}}^2 + u_{\text{tran}}^2 + u_{\text{homo}}^2 + u_{\text{its}}^2)^{1/2}$ where u_i are the individual uncertainty components for manufacturing, transportation, homogeneity, and shelf life. While no significant uncertainty was detected in the replicates, a minimum contribution to

Manufactured By:



Jared Ball

1 -Jul-2021

Production Chemist I

Certified By:



Claire Desrochers

7 -Jul-2021

Quality Control Chemist I

Released By:



Susan Mathews

8 -Jul-2021

Quality Control Team Lead

7290B Investment Drive • North Charleston, SC 29418
Phone: 866.272.0932 • Fax: 866.509.5146 www.o2si.com

Certificate of Analysis

Catalog No. G34-120070-04-SS

Lot No. 454407

Expiration Date 1-Jul-2023

uncertainty was added for homogeneity and long term stability as described in ISO Guide 35:2017.

Expiration Information:

The stability of this product is based upon rigorous short term and long term testing of the solution for the certified value. These tests include the effect of temperature and packaging on the product. Studies on the short term instability have determined no contribution to instability as observed on the concentration under controlled transportation conditions. This standard is guaranteed until 1-Jul-2023

Quality Standard Documentation:

- ISO/IEC 17025:2017 "General Requirements for the Competence of Testing and Calibration" - Chemical Testing - Accredited A2LA Certificate Number 3031.01
- ISO 17034:2016 "General Requirements for the Competence of Reference Material Producers" - Reference Material Production - Accredited A2LA Certificate Number 3031.02


Manufactured By:



Jared Ball
1-Jul-2021

Production Chemist I

Certified By:



Claire Desrochers
7-Jul-2021

Quality Control Chemist I

Released By:



Susan Mathews
8-Jul-2021

Quality Control Team Lead

7290B Investment Drive • North Charleston, SC 29418
Phone: 866.272.0932 • Fax: 866.509.5146 www.o2si.com

Method 8015C - DAI Glycols

Glycols -Direct Injection (GC/FID) -
Method 8015C

FORM III
GC SEMI VOA LAB CONTROL SAMPLE RECOVERY

Lab Name: Eurofins Savannah Job No.: 580-124266-1
 SDG No.: _____
 Matrix: Water Level: Low Lab File ID: GC07021.D
 Lab ID: LCS 680-766428/13 Client ID: _____

COMPOUND	SPIKE ADDED (mg/L)	LCS CONCENTRATION (mg/L)	LCS % REC	QC LIMITS REC	#
2-(2-Butoxyethoxy) ethanol	20.0	21.5	107	50-150	

Column to be used to flag recovery and RPD values
 FORM III 8015C GLY

FORM III
GC SEMI VOA LAB CONTROL SAMPLE DUPLICATE RECOVERY

Lab Name: Eurofins Savannah Job No.: 580-124266-1
 SDG No.: _____
 Matrix: Water Level: Low Lab File ID: GC07022.D
 Lab ID: LCSD 680-766428/14 Client ID: _____

COMPOUND	SPIKE ADDED (mg/L)	LCSD CONCENTRATION (mg/L)	LCSD % REC	% RPD	QC LIMITS		#
					RPD	REC	
2-(2-Butoxyethoxy) ethanol	20.0	23.1	116	7	50	50-150	

Column to be used to flag recovery and RPD values
 FORM III 8015C GLY

FORM III
GC SEMI VOA MATRIX SPIKE RECOVERY

Lab Name: Eurofins Savannah Job No.: 580-124266-1

SDG No.: _____

Matrix: Water Level: Low Lab File ID: GC07045.D

Lab ID: 580-124266-2 MS Client ID: AF-RHMW02-WGN01LF-2302W4 MS

COMPOUND	SPIKE ADDED (mg/L)	SAMPLE CONCENTRATION (mg/L)	MS CONCENTRATION (mg/L)	MS % REC	QC LIMITS REC	#
2-(2-Butoxyethoxy) ethanol	20.0	3.0 U	26.0	130	50-150	

Column to be used to flag recovery and RPD values

FORM III
GC SEMI VOA MATRIX SPIKE DUPLICATE RECOVERY

Lab Name: Eurofins Savannah Job No.: 580-124266-1

SDG No.: _____

Matrix: Water Level: Low Lab File ID: GC07046.D

Lab ID: 580-124266-2 MSD Client ID: AF-RHMW02-WGN01LF-2302W4 MSD

COMPOUND	SPIKE ADDED (mg/L)	MSD CONCENTRATION (mg/L)	MSD % REC	% RPD	QC LIMITS		#
					RPD	REC	
2-(2-Butoxyethoxy) ethanol	20.0	28.2	141	8	50	50-150	

Column to be used to flag recovery and RPD values

FORM IV
GC SEMI VOA METHOD BLANK SUMMARY

Lab Name: Eurofins Savannah Job No.: 580-124266-1
 SDG No.: _____
 Lab Sample ID: MB 680-766428/17
 Matrix: Water Date Extracted: _____
 Lab File ID: (1) GC07025.D Lab File ID: (2) _____
 Date Analyzed: (1) 03/07/2023 22:18 Date Analyzed: (2) _____
 Instrument ID: (1) CVGG2 Instrument ID: (2) _____
 GC Column: (1) J&W DB WAX ID: 0.45 (mm) GC Column: (2) _____ ID: _____

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES:

CLIENT SAMPLE ID	LAB SAMPLE ID	DATE ANALYZED 1	DATE ANALYZED 2
	LCS 680-766428/13	03/07/2023 20:44	
	LCSD 680-766428/14	03/07/2023 21:07	
AF-RHMW03-WGN01LF-2302W4	580-124266-1	03/08/2023 05:18	
AF-RHMW02-WGN01LF-2302W4	580-124266-2	03/08/2023 05:42	
AF-RHMW02-WGN01LF-2302W4 MS	580-124266-2 MS	03/08/2023 06:05	
AF-RHMW02-WGN01LF-2302W4 MSD	580-124266-2 MSD	03/08/2023 06:28	

FORM VIII
GC SEMI VOA INTERNAL STANDARD AREA AND RETENTION TIME SUMMARY

Lab Name: Eurofins Savannah Job No.: 580-124266-1
 SDG No.: _____
 Sample No.: ICIS 680-766428/8 Date Analyzed: 03/07/2023 18:46
 Instrument ID: CVGG2 GC Column: J&W DB WAX ID: 0.45 (mm)
 Lab File ID (Standard): GC07016.D Heated Purge: (Y/N) N
 Calibration ID: 90044

		nHPA					
		AREA #	RT #	#	RT #	#	RT #
INITIAL CALIBRATION MID-POINT		7374106	4.20				
UPPER LIMIT		14748212	4.70				
LOWER LIMIT		3687053	3.70				
LAB SAMPLE ID	CLIENT SAMPLE ID						
ICV 680-766428/12 CCV		5894548	4.20				
LCS 680-766428/13		5749580	4.20				
LCSD 680-766428/14		5861610	4.20				
MB 680-766428/17		6806623	4.20				
CCV 680-766428/32		6126690	4.20				
580-124266-1	AF-RHMW03-WGN01LF-2 302W4	6011713	4.20				
580-124266-2	AF-RHMW02-WGN01LF-2 302W4	6152301	4.19				
580-124266-2 MS	AF-RHMW02-WGN01LF-2 302W4 MS	6223277	4.20				
580-124266-2 MSD	AF-RHMW02-WGN01LF-2 302W4 MSD	6337151	4.19				
CCV 680-766428/40		6469378	4.20				

nHPA = n-Heptyl Alcohol

Area Limit = 50%-200% of internal standard area
 RT Limit = ± 0.5 minutes of internal standard RT

Column used to flag values outside QC limits

FORM I
GC SEMI VOA ORGANICS ANALYSIS DATA SHEET

Lab Name: Eurofins Savannah Job No.: 580-124266-1
 SDG No.: _____
 Client Sample ID: AF-RHMW03-WGN01LF-2302W4 Lab Sample ID: 580-124266-1
 Matrix: Water Lab File ID: GC07043.D
 Analysis Method: 8015C GLY Date Collected: 03/02/2023 12:45
 Extraction Method: _____ Date Extracted: _____
 Sample wt/vol: 1(mL) Date Analyzed: 03/08/2023 05:18
 Con. Extract Vol.: 1(mL) Dilution Factor: 1
 Injection Volume: 1(uL) GC Column: J&W DB WAX ID: 0.45(mm)
 % Moisture: _____ % Solids: _____ GPC Cleanup: (Y/N) N
 Cleanup Factor: _____
 Analysis Batch No.: 766428 Units: mg/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
112-34-5	2-(2-Butoxyethoxy)ethanol	3.0	U M	5.0	3.0	1.1

Eurofins Savannah
Target Compound Quantitation Report

Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07043.D
 Lims ID: 580-124266-A-1
 Client ID: AF-RHMW03-WGN01LF-2302W4
 Sample Type: Client
 Inject. Date: 08-Mar-2023 05:18:57 ALS Bottle#: 0 Worklist Smp#: 35
 Injection Vol: 1.0 ul Dil. Factor: 1.0000
 Sample Info: 680-0084239-035
 Operator ID: Instrument ID: CVGG2
 Method: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\8015_GLY_VGG.m
 Limit Group: 8015C_DAI
 Last Update: 08-Mar-2023 11:26:45 Calib Date: 07-Mar-2023 19:57:23
 Integrator: Falcon
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07019.D
 Column 1 : J&W DB WAX (0.45 mm) Det: GC FID2B
 Process Host: CTX1619

First Level Reviewer: SWK1 Date: 08-Mar-2023 11:20:18

RT (min.)	Exp RT (min.)	Dlt RT (min.)	Response	OnCol Amt ug/ml	Flags
--------------	------------------	------------------	----------	--------------------	-------

* 4 n-Heptyl Alcohol
 4.197 4.204 -0.007 6011713 50.0

QC Flag Legend

Processing Flags

Reagents:

SG_GLY_ISTD_00106 Amount Added: 10.00 Units: uL Run Reagent

Eurofins Savannah

Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07043.D

Injection Date: 08-Mar-2023 05:18:57

Instrument ID: CVGG2

Operator ID:

Lims ID: 580-124266-A-1

Lab Sample ID: 680-124266-1

Worklist Smp#: 35

Client ID: AF-RHMMW03-WGN01LF-2302W4

Injection Vol: 1.0 ul


Dil. Factor: 1.0000

ALS Bottle#: 0

Method: 8015_GLY_VGG

Limit Group: 8015C_DAI

Column: J&W DB WAX (0.45 mm)

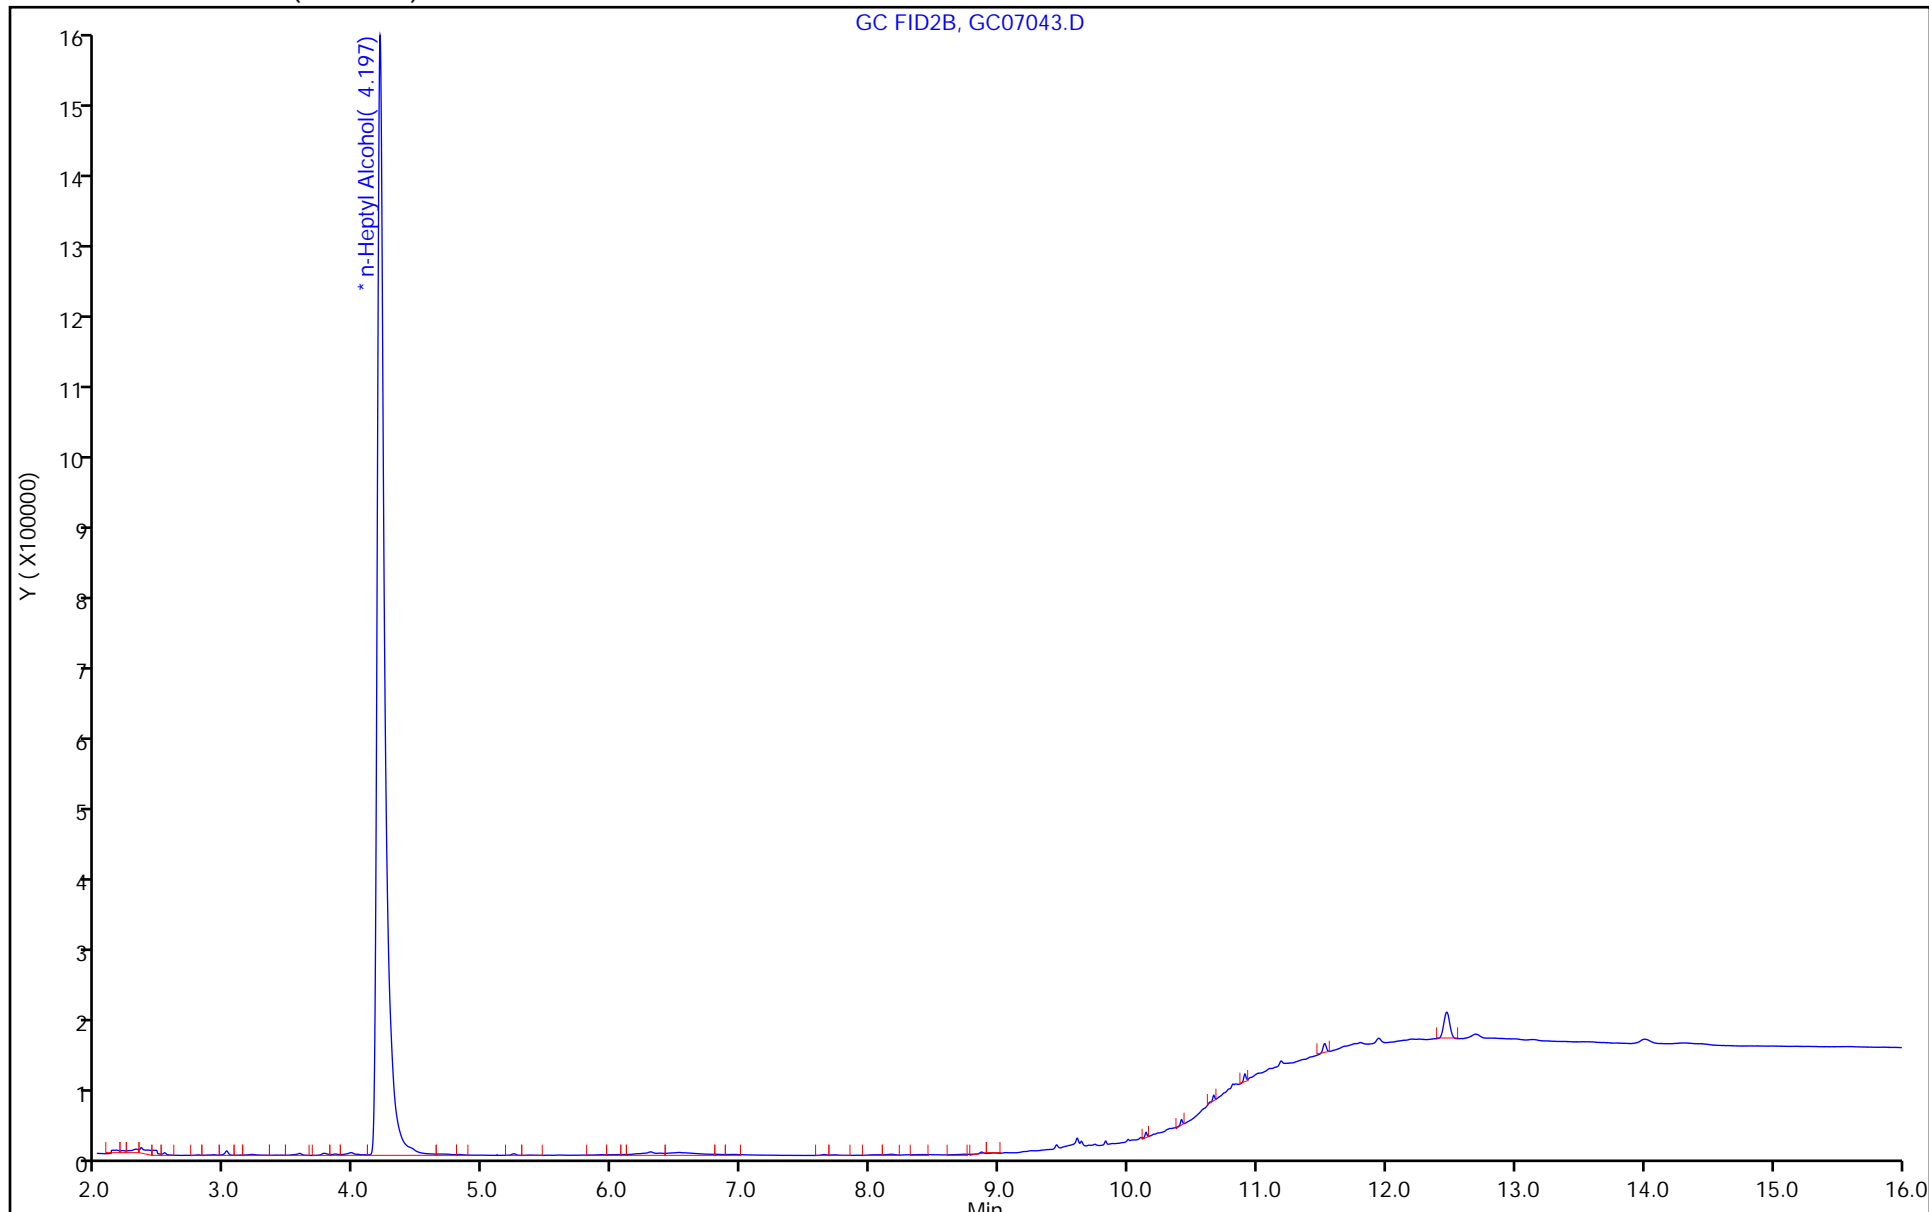

GC FID2B, GC07043.D

FORM I
GC SEMI VOA ORGANICS ANALYSIS DATA SHEET

Lab Name: Eurofins Savannah Job No.: 580-124266-1
 SDG No.: _____
 Client Sample ID: AF-RHMMW02-WGN01LF-2302W4 Lab Sample ID: 580-124266-2
 Matrix: Water Lab File ID: GC07044.D
 Analysis Method: 8015C GLY Date Collected: 03/02/2023 11:10
 Extraction Method: _____ Date Extracted: _____
 Sample wt/vol: 1(mL) Date Analyzed: 03/08/2023 05:42
 Con. Extract Vol.: 1(mL) Dilution Factor: 1
 Injection Volume: 1(uL) GC Column: J&W DB WAX ID: 0.45(mm)
 % Moisture: _____ % Solids: _____ GPC Cleanup: (Y/N) N
 Cleanup Factor: _____
 Analysis Batch No.: 766428 Units: mg/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
112-34-5	2-(2-Butoxyethoxy)ethanol	3.0	U M	5.0	3.0	1.1

Eurofins Savannah
Target Compound Quantitation Report

Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07044.D
 Lims ID: 580-124266-A-2
 Client ID: AF-RHMW02-WGN01LF-2302W4
 Sample Type: Client
 Inject. Date: 08-Mar-2023 05:42:13 ALS Bottle#: 0 Worklist Smp#: 36
 Injection Vol: 1.0 ul Dil. Factor: 1.0000
 Sample Info: 680-0084239-036
 Operator ID: Instrument ID: CVGG2

Method: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\8015_GLY_VGG.m
 Limit Group: 8015C_DAI
 Last Update: 08-Mar-2023 11:26:45 Calib Date: 07-Mar-2023 19:57:23
 Integrator: Falcon
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07019.D
 Column 1 : J&W DB WAX (0.45 mm) Det: GC FID2B
 Process Host: CTX1619

First Level Reviewer: SWK1 Date: 08-Mar-2023 11:20:31

RT (min.)	Exp RT (min.)	Dlt RT (min.)	Response	OnCol Amt ug/ml	Flags
--------------	------------------	------------------	----------	--------------------	-------

* 4 n-Heptyl Alcohol
 4.194 4.204 -0.010 6152301 50.0

QC Flag Legend

Processing Flags

Reagents:

SG_GLY_ISTD_00106 Amount Added: 10.00 Units: uL Run Reagent

Eurofins Savannah

Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07044.D

Injection Date: 08-Mar-2023 05:42:13

Instrument ID: CVGG2

Operator ID:

Lims ID: 580-124266-A-2

Lab Sample ID: 680-124266-2

Worklist Smp#: 36

Client ID: AF-RHMMW02-WGN01LF-2302W4

Injection Vol: 1.0 ul


Dil. Factor: 1.0000

ALS Bottle#: 0

Method: 8015_GLY_VGG

Limit Group: 8015C_DAI

Column: J&W DB WAX (0.45 mm)

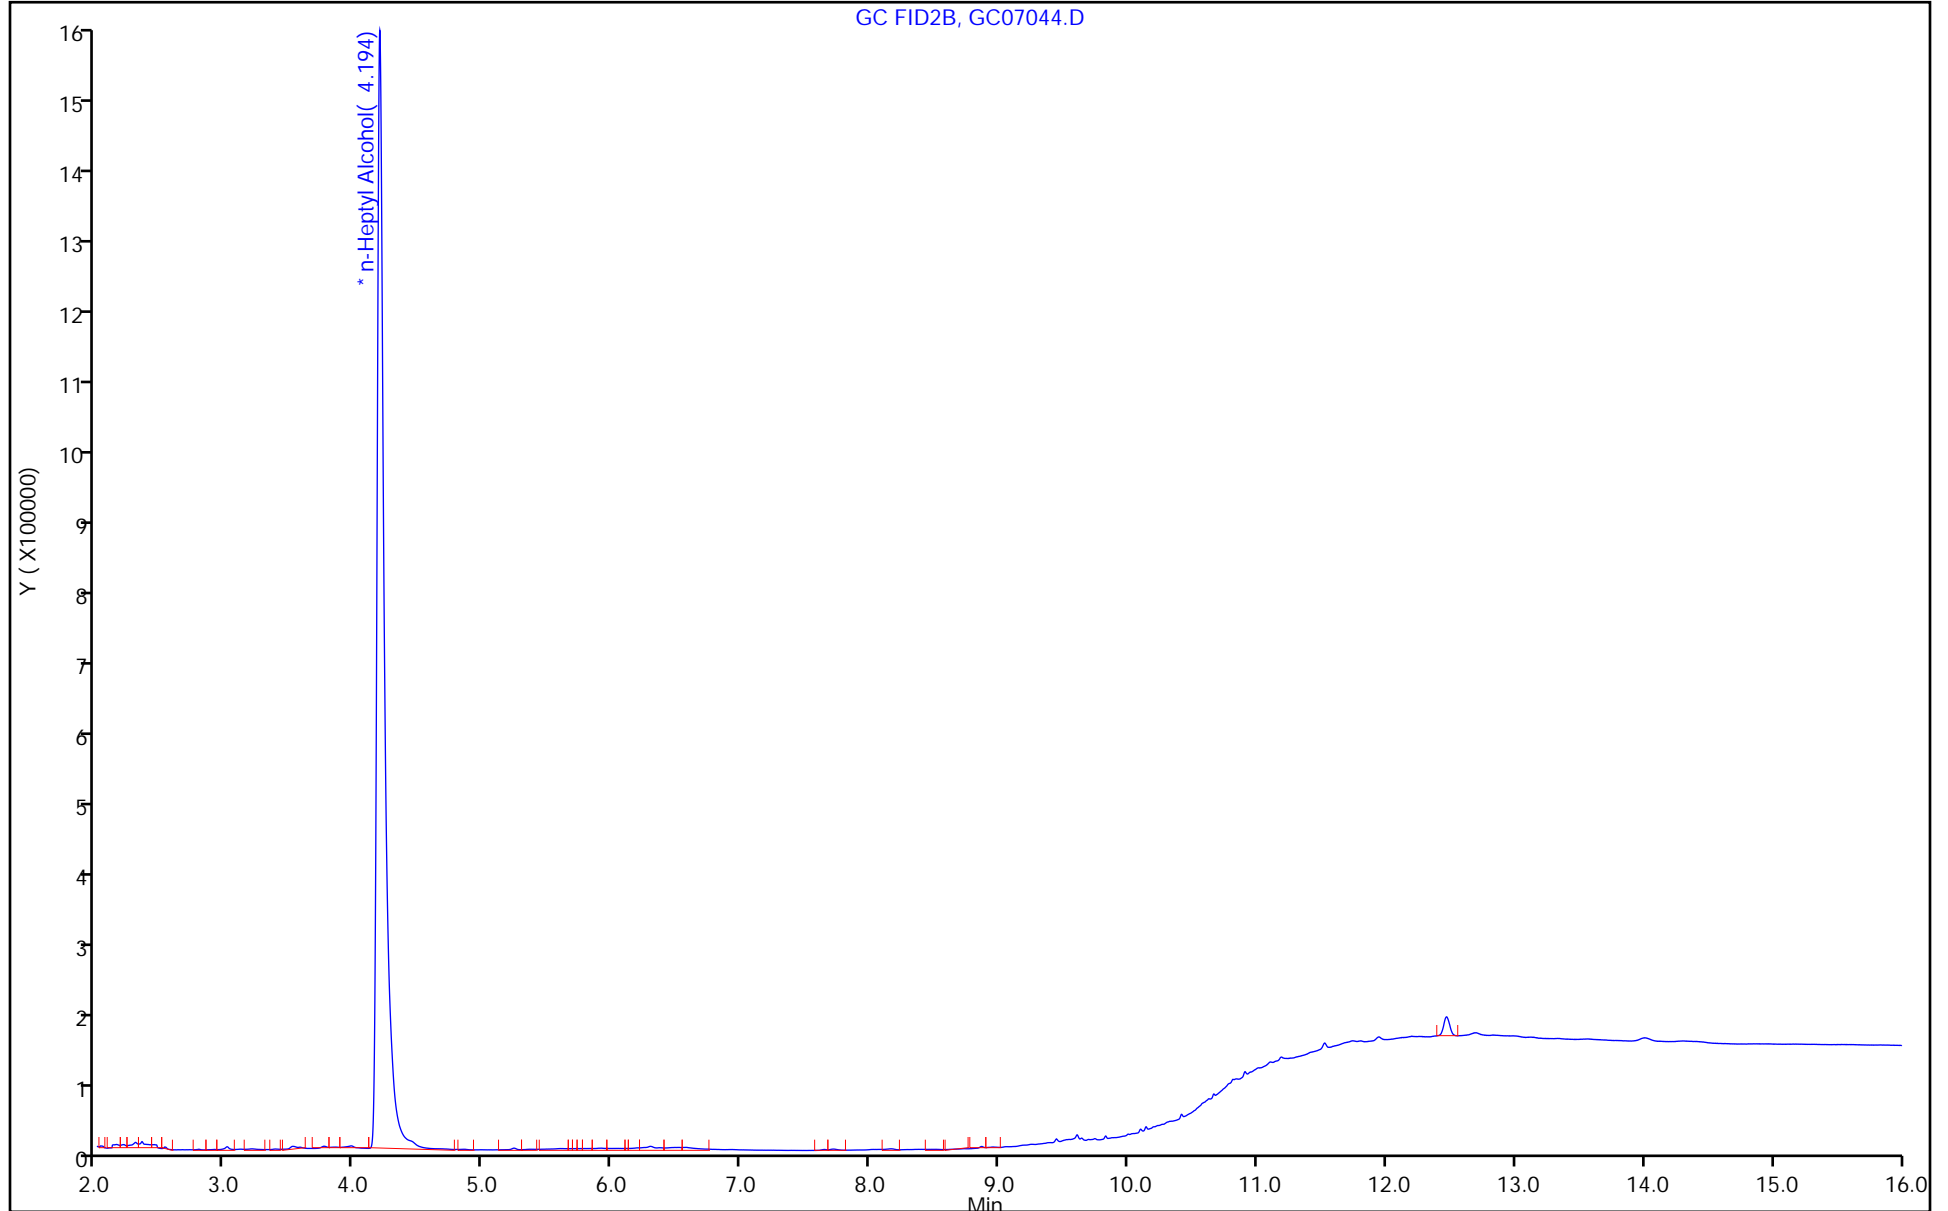

GC FID2B, GC07044.D

FORM VI
GC SEMI VOA BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
CURVE EVALUATION

Lab Name: Eurofins Savannah Job No.: 580-124266-1 Analy Batch No.: 766428

SDG No.: _____

Instrument ID: CVGG2 GC Column: J&W DB WAX ID: 0.45 (mm) Heated Purge: (Y/N) N

Calibration Start Date: 03/07/2023 17:36 Calibration End Date: 03/07/2023 19:57 Calibration ID: 90044

Calibration Files

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 680-766428/11	GC07019.D
Level 2	IC 680-766428/10	GC07018.D
Level 3	IC 680-766428/9	GC07017.D
Level 4	ICIS 680-766428/8	GC07016.D
Level 5	IC 680-766428/7	GC07015.D
Level 6	IC 680-766428/6	GC07014.D
Level 7	IC 680-766428/5	GC07013.D

ANALYTE	RRF					CURVE TYPE	COEFFICIENT			#	MIN RRF	%RSD /RSE	#	MAX %RSD /RSE	R^2 OR COD	#	MIN R^2 OR COD
	LVL 1	LVL 2	LVL 3	LVL 4	LVL 5		B	M1	M2								
	LVL 6	LVL 7															
Ethanol, 2-propoxy	1.1159 ++++	0.8566 0.4926	0.6419	++++	0.5770	Lin1	1.408 2	0.503 0						0.9940		0.9900	
4-Hydroxy-4-methyl-2-pentanone	1.0742 ++++	0.8423 0.4636	0.5868	++++	0.5367	Lin1	1.390 7	0.469 9						0.9940		0.9900	
2-Butoxyethanol	1.2395 ++++	0.9291 0.5480	0.7202	++++	0.6384	Lin2	1.348 0	0.591 3						0.9910		0.9900	
Dipropylene Glycol Methyl Ether	0.0769 ++++	0.0607 0.0369	0.0442	++++	0.0413	Lin1	0.089 4	0.037 2						0.9970		0.9900	
Propylene glycol	0.2567 ++++	0.1675 0.1348	0.1804	++++	0.1442	Lin1	0.249 2	0.135 4						0.9970		0.9900	
Ethylene glycol	0.4941 ++++	0.3710 0.3728	0.5274	++++	0.3852	Lin1	0.315 5	0.377 7						0.9910		0.9900	
2-(2-Butoxyethoxy)ethanol	0.9509 ++++	0.6750 0.4032	0.5224	++++	0.4510	Lin2	1.089 7	0.419 6						0.9950		0.9900	
2,2'-Oxybisethanol	0.4429 ++++	0.2099 0.2304	0.3012	++++	0.2467	Lin1	0.329 0	0.231 6						0.9920		0.9900	
Triethylene Glycol	0.4632 ++++	0.2141 0.2249	0.3027	++++	0.2346	Lin1	0.388 8	0.223 4						0.9910		0.9900	
Tetraethylene Glycol	0.4337 ++++	0.1983 0.2296	0.3036	++++	0.2366	Lin1	0.628 1	0.228 2						0.9910		0.9900	

Note: The M1 coefficient is the same as Ave RRF for an Ave curve type. RSD is calculated for Ave curve types. RSE is used for all other types.

FORM VI
GC SEMI VOA BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
RESPONSE AND CONCENTRATION

Lab Name: Eurofins Savannah Job No.: 580-124266-1 Analy Batch No.: 766428

SDG No.: _____

Instrument ID: CVGG2 GC Column: J&W DB WAX ID: 0.45 (mm) Heated Purge: (Y/N) N

Calibration Start Date: 03/07/2023 17:36 Calibration End Date: 03/07/2023 19:57 Calibration ID: 90044

Calibration Files

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 680-766428/11	GC07019.D
Level 2	IC 680-766428/10	GC07018.D
Level 3	IC 680-766428/9	GC07017.D
Level 4	ICIS 680-766428/8	GC07016.D
Level 5	IC 680-766428/7	GC07015.D
Level 6	IC 680-766428/6	GC07014.D
Level 7	IC 680-766428/5	GC07013.D

ANALYTE	IS REF	CURVE TYPE	RESPONSE					CONCENTRATION (UG/ML)				
			LVL 1 LVL 6	LVL 2 LVL 7	LVL 3	LVL 4	LVL 5	LVL 1 LVL 6	LVL 2 LVL 7	LVL 3	LVL 4	LVL 5
Ethanol, 2-propoxy	nHPA	Lin1	258368 ++++	460254 5169931	777408	++++	2589037	2.00 ++++	5.00 100	10.0	++++	50.0
4-Hydroxy-4-methyl-2-pentanone	nHPA	Lin1	248723 ++++	452575 4864934	710717	++++	2408106	2.00 ++++	5.00 100	10.0	++++	50.0
2-Butoxyethanol	nHPA	Lin2	286987 ++++	499197 5750395	872287	++++	2864549	2.00 ++++	5.00 100	10.0	++++	50.0
Dipropylene Glycol Methyl Ether	nHPA	Lin1	17808 ++++	32612 387288	53581	++++	185288	2.00 ++++	5.00 100	10.0	++++	50.0
Propylene glycol	nHPA	Lin1	59431 ++++	90003 1414987	218465	++++	647209	2.00 ++++	5.00 100	10.0	++++	50.0
Ethylene glycol	nHPA	Lin1	114413 ++++	199343 3912634	638794	++++	1728270	2.00 ++++	5.00 100	10.0	++++	50.0
2-(2-Butoxyethoxy)ethanol	nHPA	Lin2	220174 ++++	362653 4231610	632720	++++	2023687	2.00 ++++	5.00 100	10.0	++++	50.0
2,2'-Oxybisethanol	nHPA	Lin1	102548 ++++	112793 2417770	364788	++++	1107173	2.00 ++++	5.00 100	10.0	++++	50.0
Triethylene Glycol	nHPA	Lin1	107241 ++++	115060 2360199	366556	++++	1052624	2.00 ++++	5.00 100	10.0	++++	50.0
Tetraethylene Glycol	nHPA	Lin1	200864 ++++	213051 4819244	735490	++++	2122943	4.00 ++++	10.0 200	20.0	++++	100

Curve Type Legend

Lin1 = Linear 1/conc ISTD
Lin2 = Linear 1/conc^2 ISTD

FORM VI
GC SEMI VOA BY INTERNAL STANDARD - INITIAL CALIBRATION DATA
READBACK PERCENT ERROR

Lab Name: Eurofins Savannah Job No.: 580-124266-1 Analy Batch No.: 766428

SDG No.: _____

Instrument ID: CVGG2 GC Column: J&W DB WAX ID: 0.45 (mm) Heated Purge: (Y/N) N

Calibration Start Date: 03/07/2023 17:36 Calibration End Date: 03/07/2023 19:57 Calibration ID: 90044

Calibration Files

LEVEL:	LAB SAMPLE ID:	LAB FILE ID:
Level 1	IC 680-766428/11	GC07019.D
Level 2	IC 680-766428/10	GC07018.D
Level 3	IC 680-766428/9	GC07017.D
Level 4	ICIS 680-766428/8	GC07016.D
Level 5	IC 680-766428/7	GC07015.D
Level 6	IC 680-766428/6	GC07014.D
Level 7	IC 680-766428/5	GC07013.D

ANALYTE	PERCENT ERROR						PERCENT ERROR LIMIT					
	LVL 1 # LVL 7 #	LVL 2 #	LVL 3 #	LVL 4 #	LVL 5 #	LVL 6 #	LVL 1 LVL 7	LVL 2	LVL 3	LVL 4	LVL 5	LVL 6
Ethanol, 2-propoxy	-18.1 -4.9	14.3	-0.4	++++	9.1	++++	20 20	20	20		20	
4-Hydroxy-4-methyl-2-pentanone	-19.4 -4.3	20.1 *	-4.7	++++	8.3	++++	20 20	20	20		20	
2-Butoxyethanol	-4.4 -9.6	11.5	-1.0	++++	3.4	++++	20 20	20	20		20	
Dipropylene Glycol Methyl Ether	-13.3 -3.1	15.2	-5.0	++++	6.3	++++	20 20	20	20		20	
Propylene glycol	-2.4 -2.2	-13.1	14.9	++++	2.9	++++	20 20	20	20		20	
Ethylene glycol	-11.0 -2.1	-18.5	31.3 *	++++	0.3	++++	20 20	20	20		20	
2-(2-Butoxyethoxy)ethanol	-3.2 -6.5	8.9	-1.5	++++	2.3	++++	20 20	20	20		20	
2,2'-Oxybisethanol	20.2 * -1.9	-37.8 *	15.8	++++	3.7	++++	20 20	20	20		20	
Triethylene Glycol	20.3 * -1.0	-38.9 *	18.1	++++	1.5	++++	20 20	20	20		20	
Tetraethylene Glycol	21.2 * -0.8	-40.7 *	19.3	++++	0.9	++++	20 20	20	20		20	

Eurofins Savannah
Target Compound Quantitation Report

Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07013.D
 Lims ID: ic g7
 Client ID:
 Sample Type: IC Calib Level: 7
 Inject. Date: 07-Mar-2023 17:36:33 ALS Bottle#: 0 Worklist Smp#: 5
 Injection Vol: 1.0 ul Dil. Factor: 1.0000
 Sample Info: 680-0084239-005
 Operator ID: Instrument ID: CVGG2
 Sublist: chrom-8015_GLY_VGG*sub2
 Method: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\8015_GLY_VGG.m
 Limit Group: 8015C_DAI
 Last Update: 08-Mar-2023 10:54:45 Calib Date: 07-Mar-2023 19:57:23
 Integrator: Falcon
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07019.D
 Column 1 : J&W DB WAX (0.45 mm) Det: GC FID2B
 Process Host: CTX1619

First Level Reviewer: SWK1 Date: 08-Mar-2023 10:47:59

RT (min.)	Exp RT (min.)	Dlt RT (min.)	Response	Cal Amt ug/ml	OnCol Amt ug/ml	Flags
1 Ethanol, 2-propoxy						
2.902	2.906	-0.004	5169931	100.0	95.1	
2 4-Hydroxy-4-methyl-2-pentanone						
3.453	3.464	-0.011	4864934	100.0	95.7	
3 2-Butoxyethanol						
3.754	3.753	0.001	5750395	100.0	90.4	
* 4 n-Heptyl Alcohol						
4.211	4.203	0.008	5247065	50.0	50.0	
5 Dipropylene Glycol Methyl Ether						
5.131	5.137	-0.006	387288	100.0	96.9	
6 Propylene glycol						
6.349	6.351	-0.002	1414987	100.0	97.8	M
7 Ethylene glycol						
6.527	6.540	-0.013	3912634	100.0	97.9	M
8 2-(2-Butoxyethoxy)ethanol						
8.412	8.411	0.001	4231610	100.0	93.5	
9 2,2'-Oxybisethanol						
9.602	9.601	0.001	2417770	100.0	98.1	
10 Triethylene Glycol						
10.628	10.627	0.001	2360199	100.0	99.0	
11 Tetraethylene Glycol						
11.763	11.762	0.001	4819244	200.0	198.5	

QC Flag Legend
Processing Flags

Review Flags

M - Manually Integrated

Reagents:

SG_Gly_CAL_00048

Amount Added: 50.00

Units: uL

SG_GLY_ISTD_00106

Amount Added: 10.00

Units: uL

Run Reagent

Eurofins Savannah

Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07013.D

Injection Date: 07-Mar-2023 17:36:33

Instrument ID: CVGG2

Operator ID:

Lims ID: ic g7

Worklist Smp#: 5

Client ID:

Injection Vol: 1.0 ul


Dil. Factor: 1.0000

ALS Bottle#: 0

Method: 8015_GLY_VGG

Limit Group: 8015C_DAI

Column: J&W DB WAX (0.45 mm)

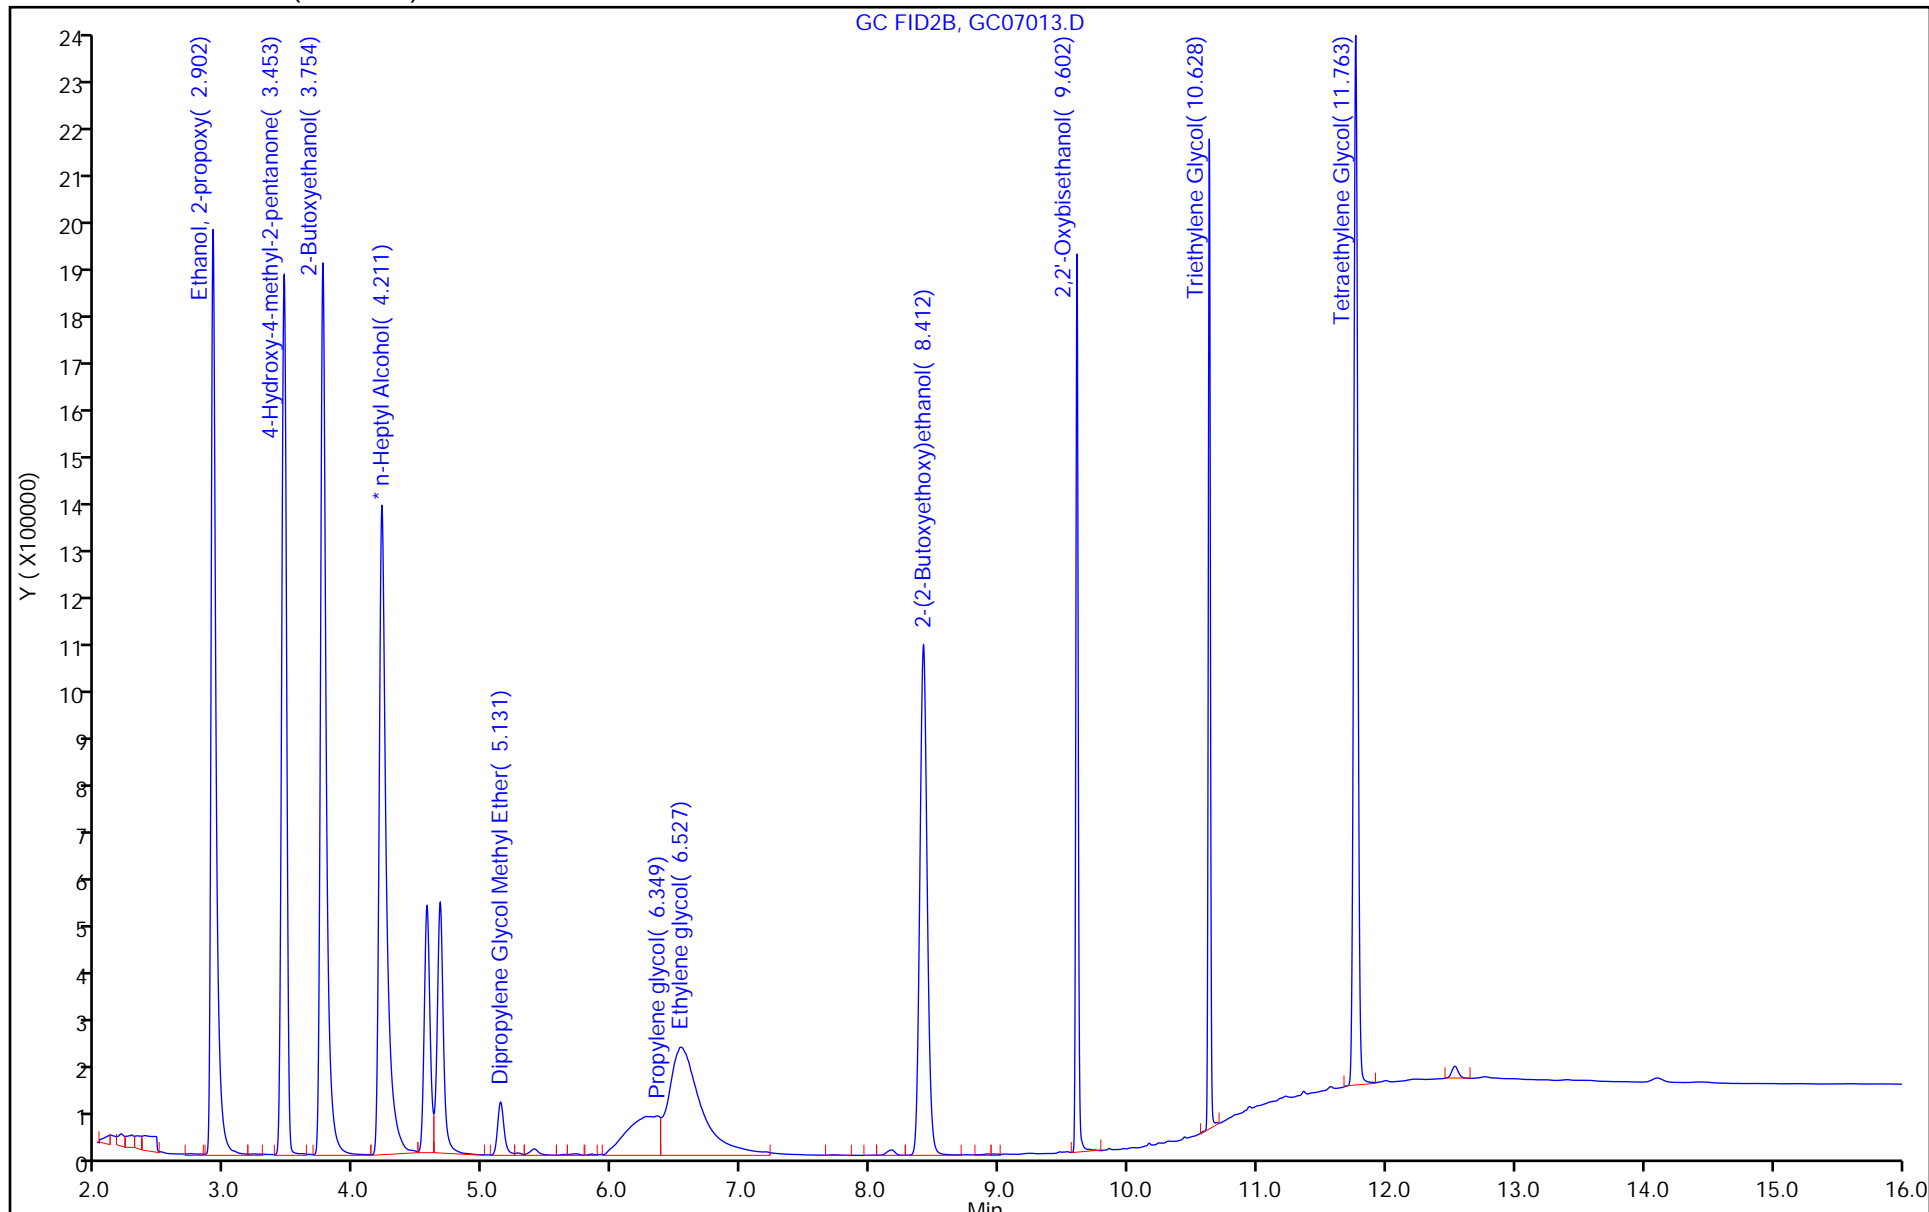

Eurofins Savannah


Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07013.D
Injection Date: 07-Mar-2023 17:36:33 Instrument ID: CVGG2
Lims ID: ic g7
Client ID:
Operator ID: ALS Bottle#: 0 Worklist Smp#: 5
Injection Vol: 1.0 ul Dil. Factor: 1.0000
Method: 8015_GLY_VGG Limit Group: 8015C_DAI
Column: J&W DB WAX (0.45 mm) Detector: GC FID2B

6 Propylene glycol, CAS: 57-55-6

Signal: 1


RT: 6.35
Area: 278872
Amount: 79.736222
Amount Units: ug/ml

Processing Integration Results

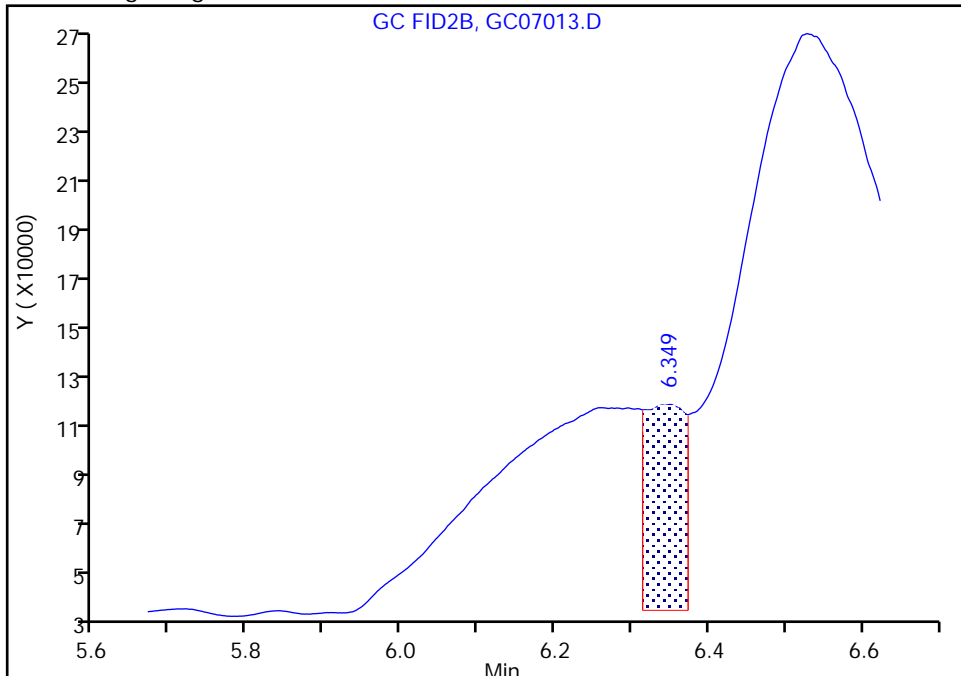

RT: 6.35
Area: 1414987
Amount: 97.776360
Amount Units: ug/ml

Manual Integration Results

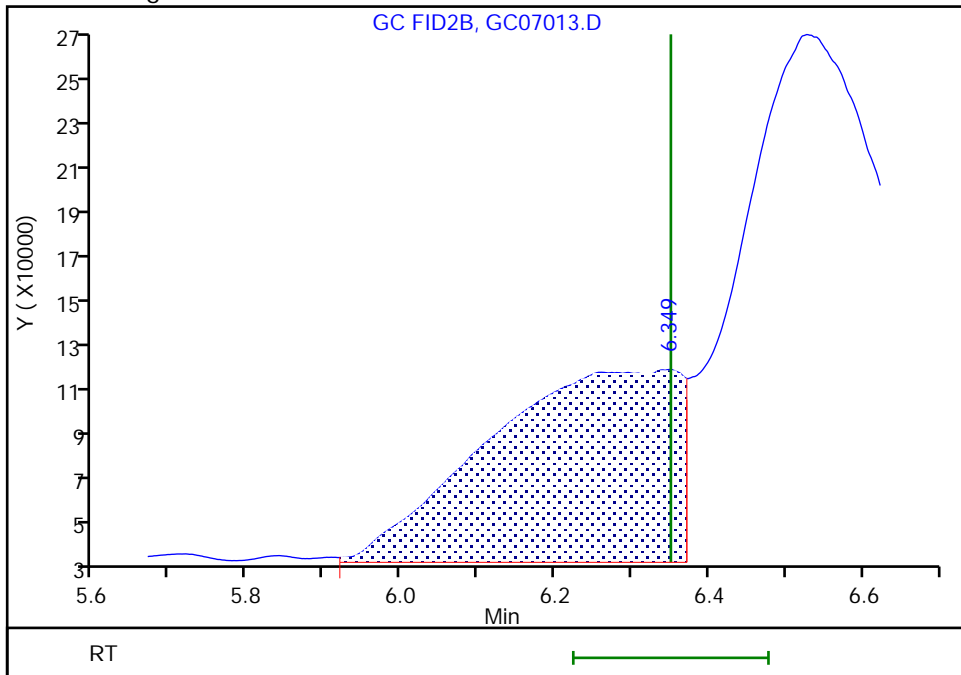

Eurofins Savannah


Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07013.D
Injection Date: 07-Mar-2023 17:36:33 Instrument ID: CVGG2
Lims ID: ic g7
Client ID:
Operator ID: ALS Bottle#: 0 Worklist Smp#: 5
Injection Vol: 1.0 ul Dil. Factor: 1.0000
Method: 8015_GLY_VGG Limit Group: 8015C_DAI
Column: J&W DB WAX (0.45 mm) Detector: GC FID2B

7 Ethylene glycol, CAS: 107-21-1

Signal: 1


RT: 6.53
Area: 3697607
Amount: 116.4421
Amount Units: ug/ml

Processing Integration Results

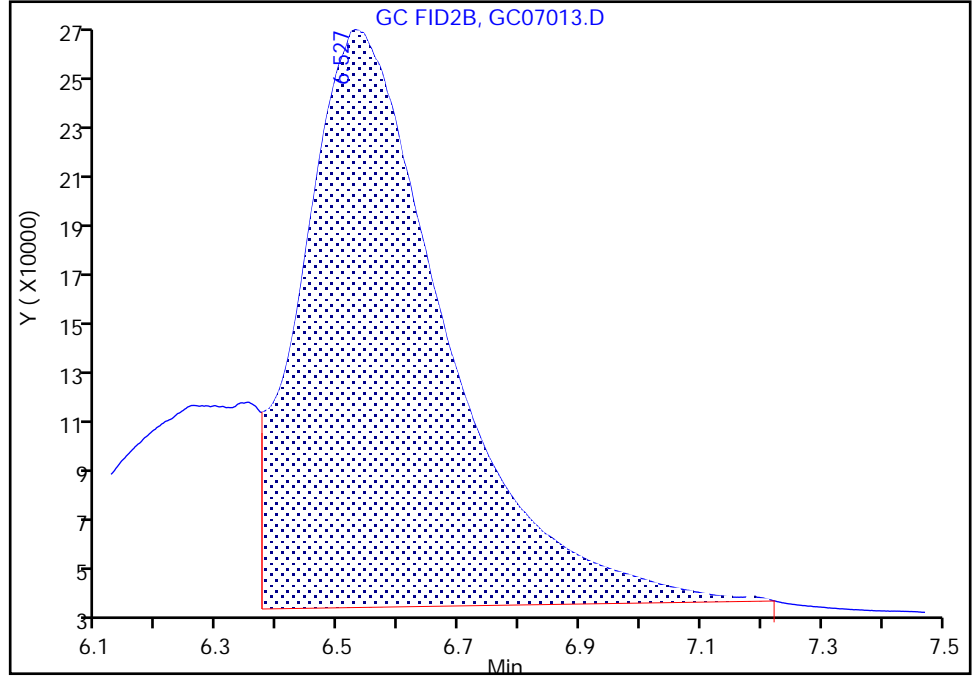

RT: 6.53
Area: 3912634
Amount: 97.867927
Amount Units: ug/ml

Manual Integration Results

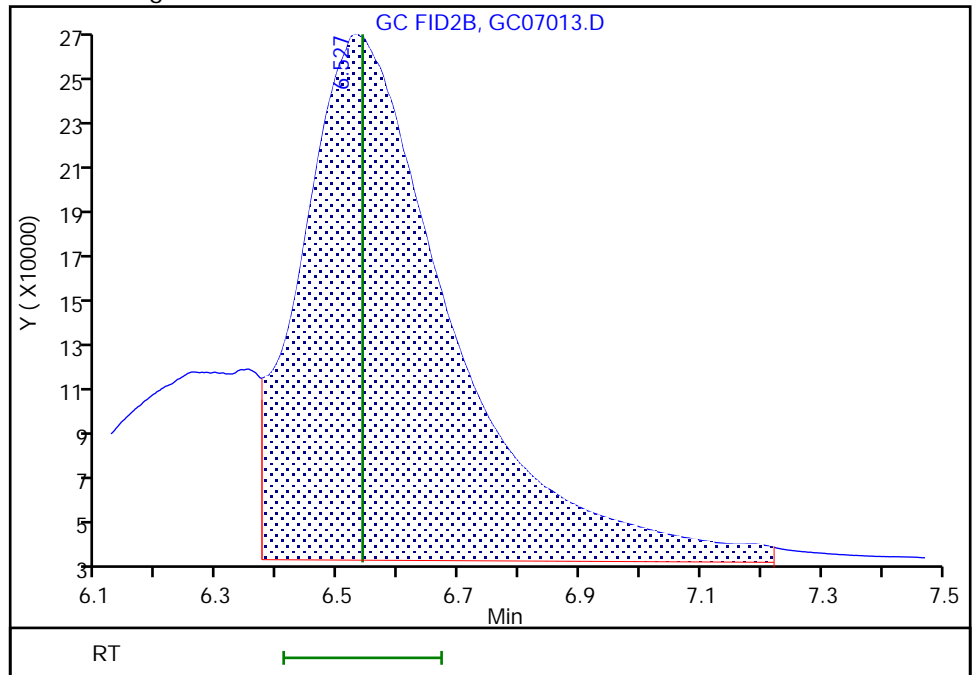

Eurofins Savannah
Target Compound Quantitation Report

Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07014.D
 Lims ID: ic g6
 Client ID:
 Sample Type: IC Calib Level: 6
 Inject. Date: 07-Mar-2023 18:00:00 ALS Bottle#: 0 Worklist Smp#: 6
 Injection Vol: 1.0 ul Dil. Factor: 1.0000
 Sample Info: 680-0084239-006
 Operator ID: Instrument ID: CVGG2
 Sublist: chrom-8015_GLY_VGG*sub2
 Method: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\8015_GLY_VGG.m
 Limit Group: 8015C_DAI
 Last Update: 08-Mar-2023 10:54:46 Calib Date: 07-Mar-2023 19:57:23
 Integrator: Falcon
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07019.D
 Column 1 : J&W DB WAX (0.45 mm) Det: GC FID2B
 Process Host: CTX1619

First Level Reviewer: SWK1 Date: 08-Mar-2023 10:48:21

RT (min.)	Exp RT (min.)	Dlt RT (min.)	Response	Cal Amt ug/ml	OnCol Amt ug/ml	Flags
1 Ethanol, 2-propoxy						
2.906	2.906	0.000	4501242	80.0	86.0	
2 4-Hydroxy-4-methyl-2-pentanone						
3.463	3.464	-0.001	4212847	80.0	86.0	
3 2-Butoxyethanol						
3.754	3.753	0.001	4884358	80.0	79.7	
* 4 n-Heptyl Alcohol						
4.205	4.203	0.002	5038257	50.0	50.0	
5 Dipropylene Glycol Methyl Ether						
5.137	5.137	0.000	314049	80.0	81.4	
6 Propylene glycol						
6.345	6.351	-0.006	868494	80.0	61.8	M
7 Ethylene glycol						
6.533	6.540	-0.007	2323608	80.0	60.2	
8 2-(2-Butoxyethoxy)ethanol						
8.410	8.411	-0.001	3243263	80.0	74.1	
9 2,2'-Oxybisethanol						
9.600	9.601	-0.001	1458800	80.0	61.1	
10 Triethylene Glycol						
10.628	10.627	0.001	1401095	80.0	60.5	
11 Tetraethylene Glycol						
11.763	11.762	0.001	2864446	160.0	121.8	

QC Flag Legend
Processing Flags

Review Flags

M - Manually Integrated

Reagents:

SG_Gly_CAL_00048

Amount Added: 40.00

Units: uL

SG_GLY_ISTD_00106

Amount Added: 10.00

Units: uL

Run Reagent

Eurofins Savannah

Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07014.D

Injection Date: 07-Mar-2023 18:00:00

Instrument ID: CVGG2

Operator ID:

Lims ID: ic g6

Worklist Smp#: 6

Client ID:

Injection Vol: 1.0 ul


Dil. Factor: 1.0000

ALS Bottle#: 0

Method: 8015_GLY_VGG

Limit Group: 8015C_DAI

Column: J&W DB WAX (0.45 mm)

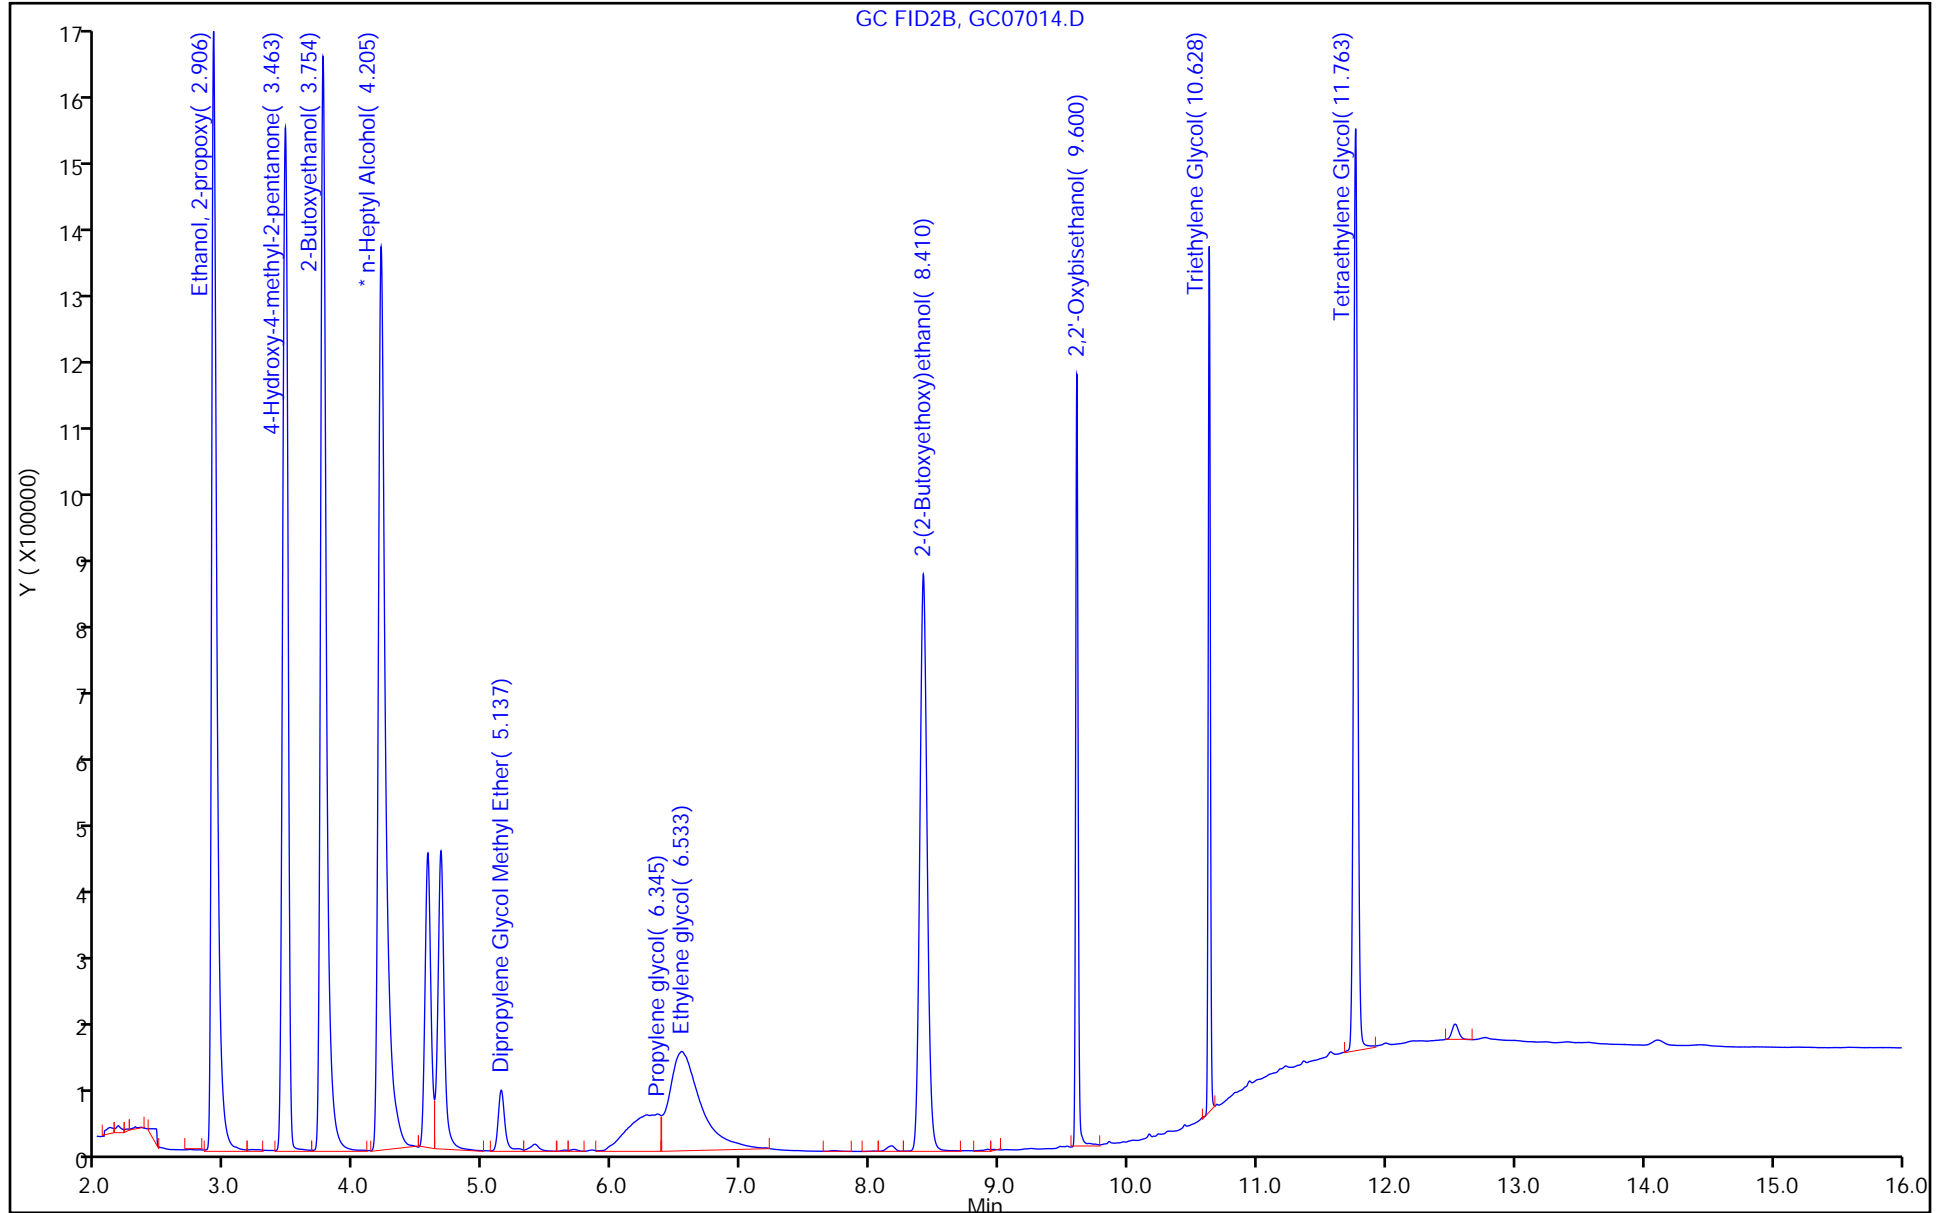

Eurofins Savannah


Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07014.D
Injection Date: 07-Mar-2023 18:00:00 Instrument ID: CVGG2
Lims ID: ic g6
Client ID:
Operator ID: ALS Bottle#: 0 Worklist Smp#: 6
Injection Vol: 1.0 ul Dil. Factor: 1.0000
Method: 8015_GLY_VGG Limit Group: 8015C_DAI
Column: J&W DB WAX (0.45 mm) Detector: GC FID2B

6 Propylene glycol, CAS: 57-55-6

Signal: 1


RT: 6.35
Area: 198531
Amount: 40.379046
Amount Units: ug/ml

Processing Integration Results

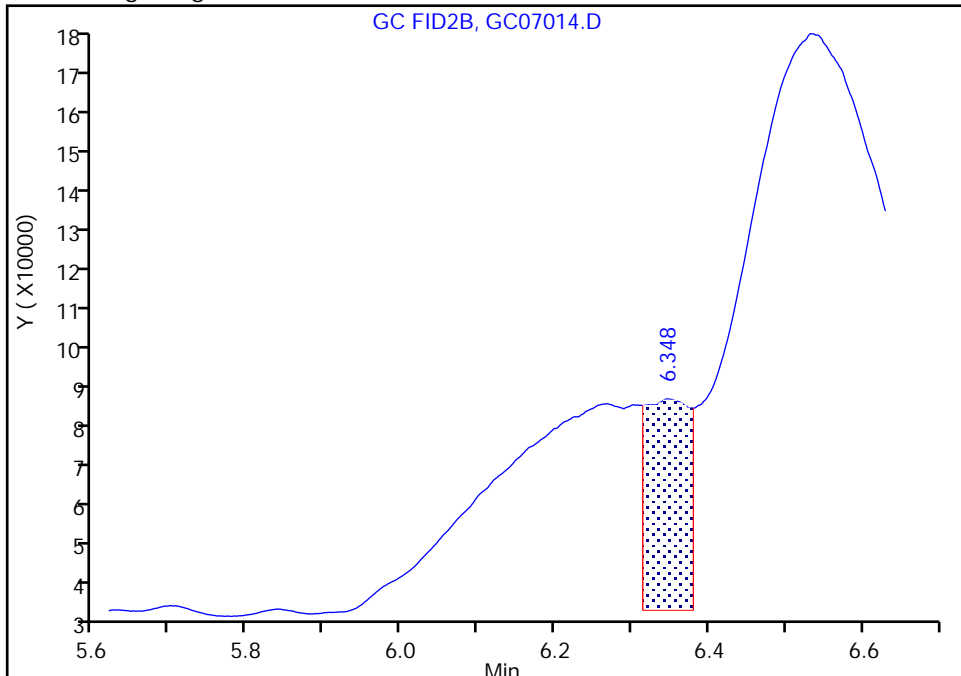

RT: 6.35
Area: 868494
Amount: 61.836268
Amount Units: ug/ml

Manual Integration Results

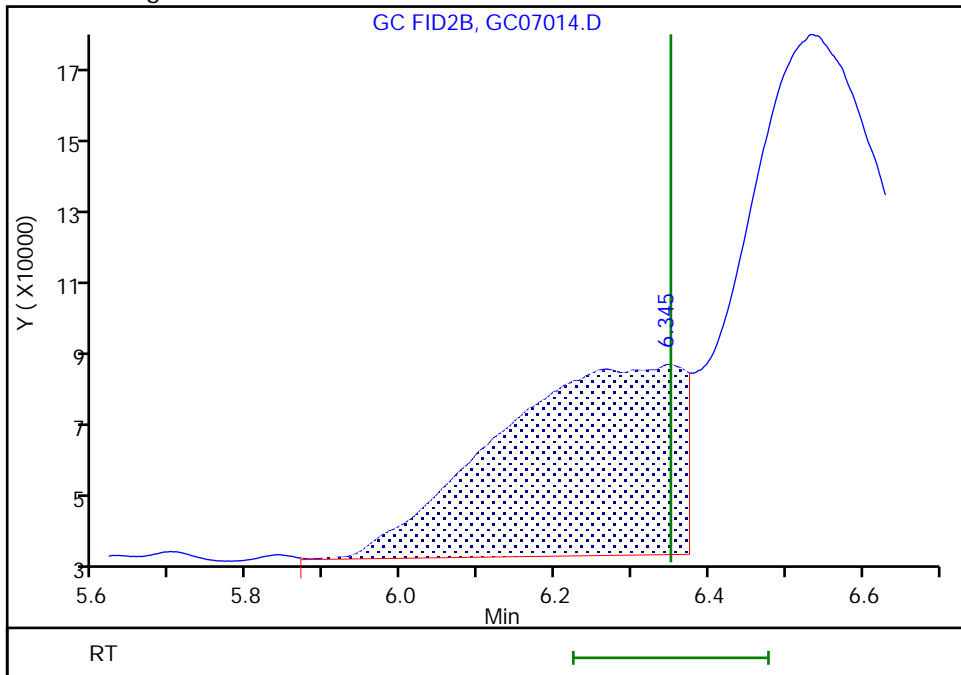

Reviewer: SWK1, 08-Mar-2023 10:48:18
Audit Action: Manually Integrated

Audit Reason: Baseline Smoothing

Eurofins Savannah
Target Compound Quantitation Report

Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07015.D
 Lims ID: ic g5
 Client ID:
 Sample Type: IC Calib Level: 5
 Inject. Date: 07-Mar-2023 18:23:27 ALS Bottle#: 0 Worklist Smp#: 7
 Injection Vol: 1.0 ul Dil. Factor: 1.0000
 Sample Info: 680-0084239-007
 Operator ID: Instrument ID: CVGG2
 Sublist: chrom-8015_GLY_VGG*sub2
 Method: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\8015_GLY_VGG.m
 Limit Group: 8015C_DAI
 Last Update: 08-Mar-2023 10:54:46 Calib Date: 07-Mar-2023 19:57:23
 Integrator: Falcon
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07019.D
 Column 1 : J&W DB WAX (0.45 mm) Det: GC FID2B
 Process Host: CTX1619

First Level Reviewer: SWK1 Date: 08-Mar-2023 10:48:29

RT (min.)	Exp RT (min.)	Dlt RT (min.)	Response	Cal Amt ug/ml	OnCol Amt ug/ml	Flags
1 Ethanol, 2-propoxy						
2.905	2.906	-0.001	2589037	50.0	54.6	
2 4-Hydroxy-4-methyl-2-pentanone						
3.459	3.464	-0.005	2408106	50.0	54.1	
3 2-Butoxyethanol						
3.754	3.753	0.001	2864549	50.0	51.7	
* 4 n-Heptyl Alcohol						
4.209	4.203	0.006	4487093	50.0	50.0	
5 Dipropylene Glycol Methyl Ether						
5.134	5.137	-0.003	185288	50.0	53.1	
6 Propylene glycol						
6.358	6.351	0.007	647209	50.0	51.4	M
7 Ethylene glycol						
6.530	6.540	-0.010	1728270	50.0	50.1	
8 2-(2-Butoxyethoxy)ethanol						
8.410	8.411	-0.001	2023687	50.0	51.1	
9 2,2'-Oxybisethanol						
9.601	9.601	0.000	1107173	50.0	51.8	
10 Triethylene Glycol						
10.628	10.627	0.001	1052624	50.0	50.8	
11 Tetraethylene Glycol						
11.763	11.762	0.001	2122943	100.0	100.9	

QC Flag Legend
Processing Flags

Review Flags

M - Manually Integrated

Reagents:

SG_Gly_CAL_00048

Amount Added: 25.00

Units: uL

SG_GLY_ISTD_00106

Amount Added: 10.00

Units: uL

Run Reagent

Eurofins Savannah

Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07015.D

Injection Date: 07-Mar-2023 18:23:27

Instrument ID: CVGG2

Operator ID:

Lims ID: ic g5

Worklist Smp#: 7

Client ID:

Injection Vol: 1.0 ul


Dil. Factor: 1.0000

ALS Bottle#: 0

Method: 8015_GLY_VGG

Limit Group: 8015C_DAI

Column: J&W DB WAX (0.45 mm)

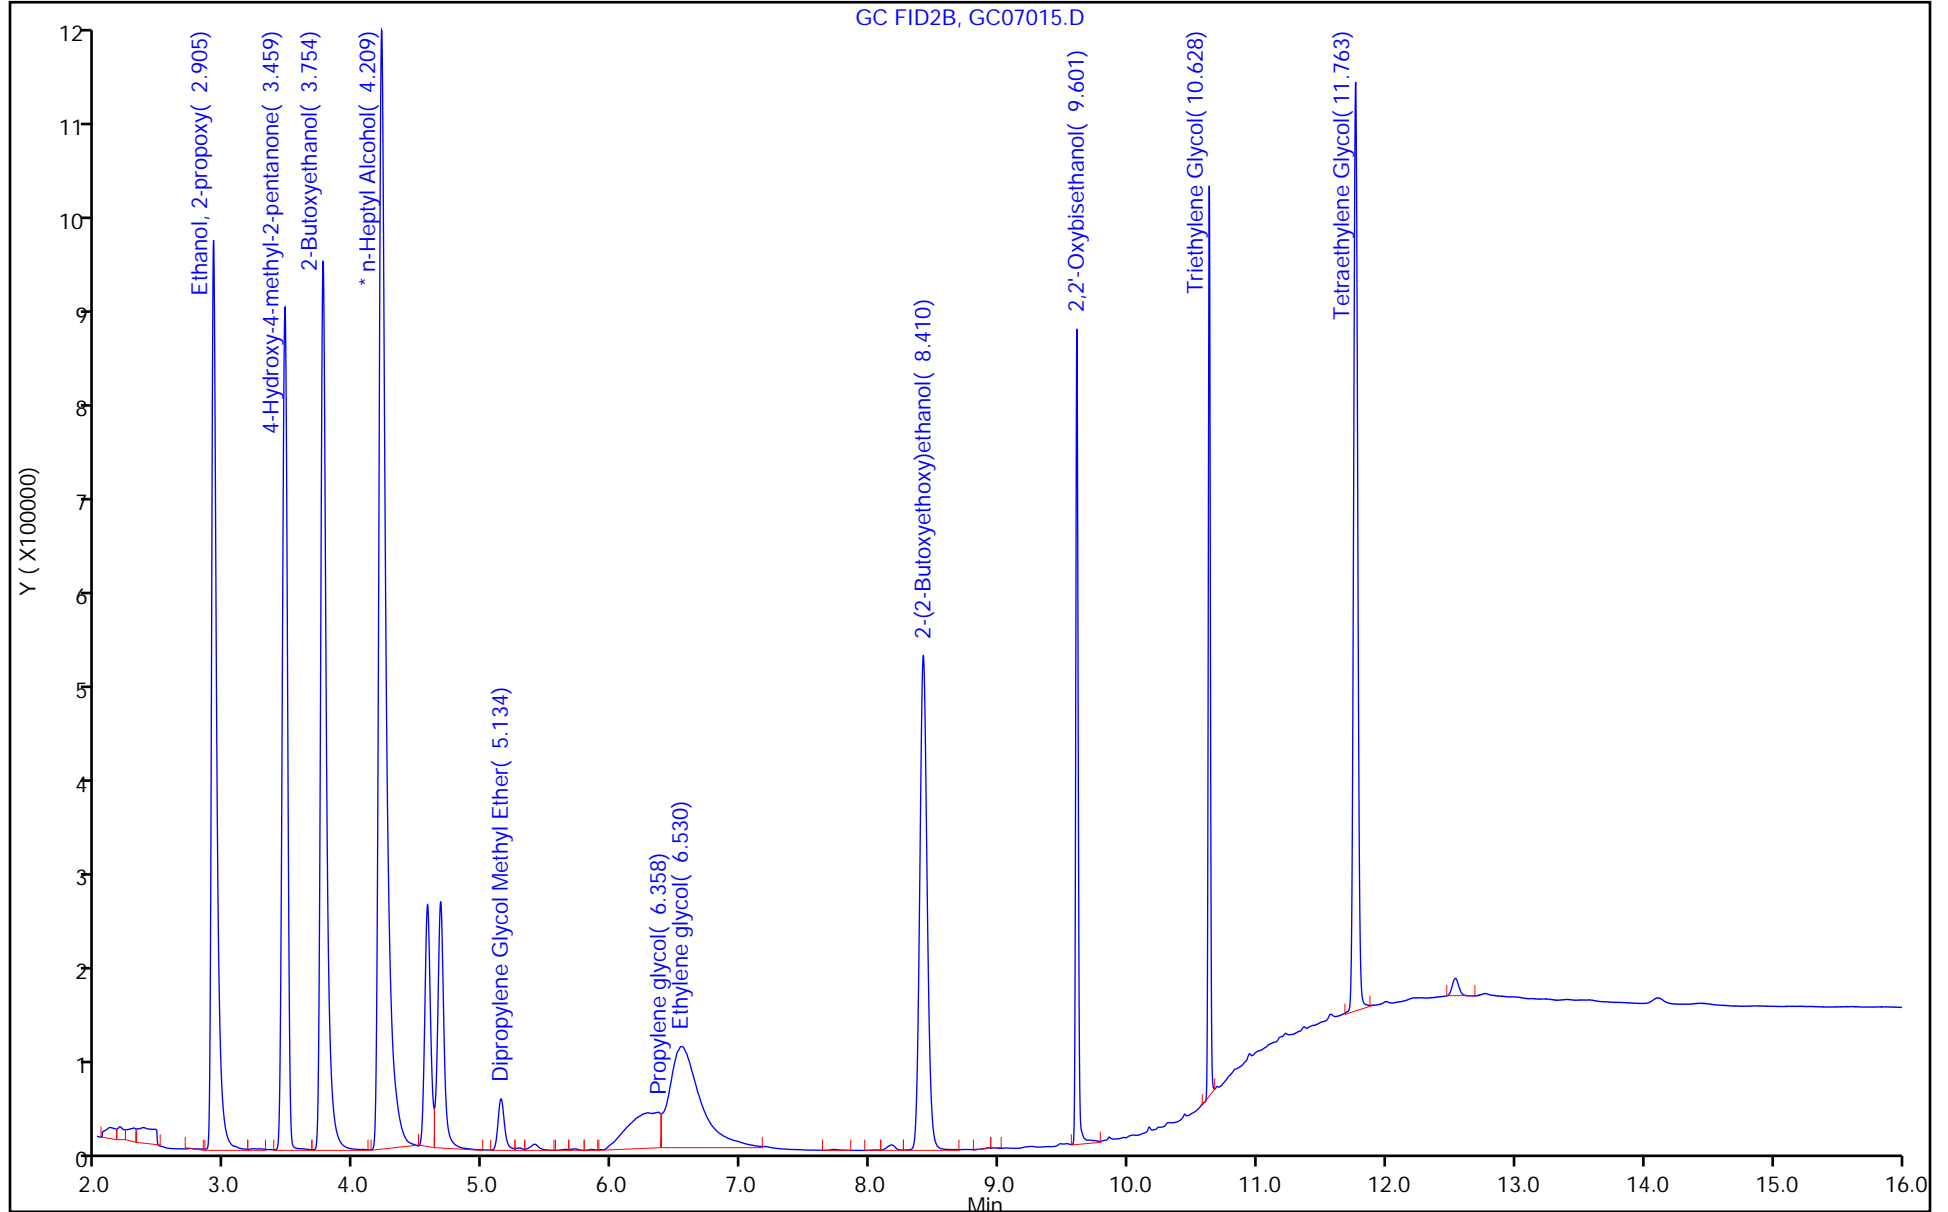

Eurofins Savannah


Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07015.D
Injection Date: 07-Mar-2023 18:23:27 Instrument ID: CVGG2
Lims ID: ic g5
Client ID:
Operator ID: ALS Bottle#: 0 Worklist Smp#: 7
Injection Vol: 1.0 ul Dil. Factor: 1.0000
Method: 8015_GLY_VGG Limit Group: 8015C_DAI
Column: J&W DB WAX (0.45 mm) Detector: GC FID2B

6 Propylene glycol, CAS: 57-55-6

Signal: 1


RT: 6.36
Area: 162601
Amount: 29.866255
Amount Units: ug/ml

Processing Integration Results

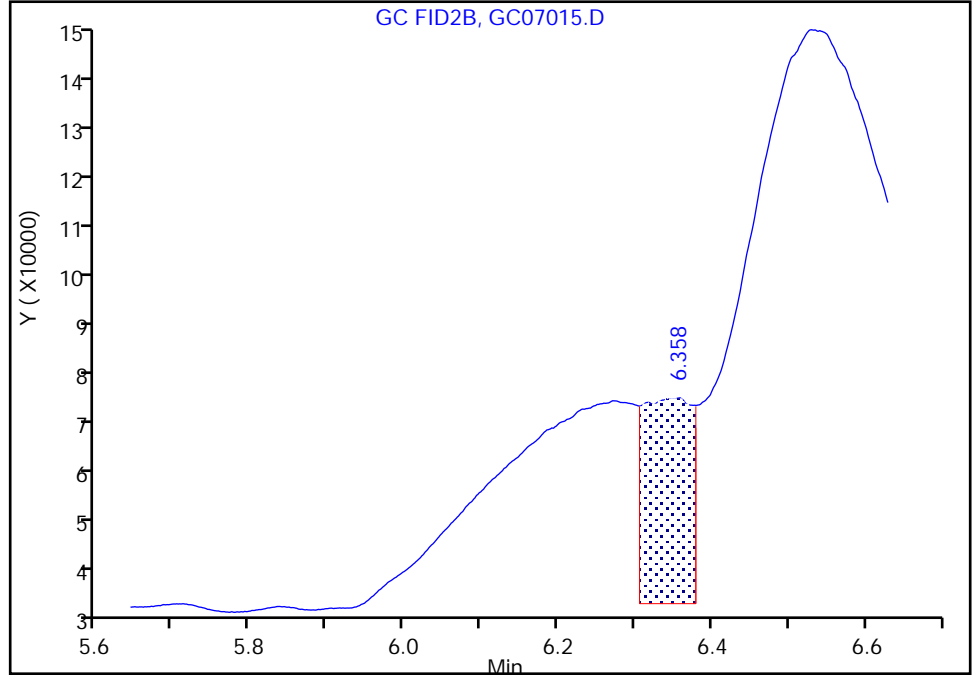

RT: 6.36
Area: 647209
Amount: 51.440544
Amount Units: ug/ml

Manual Integration Results

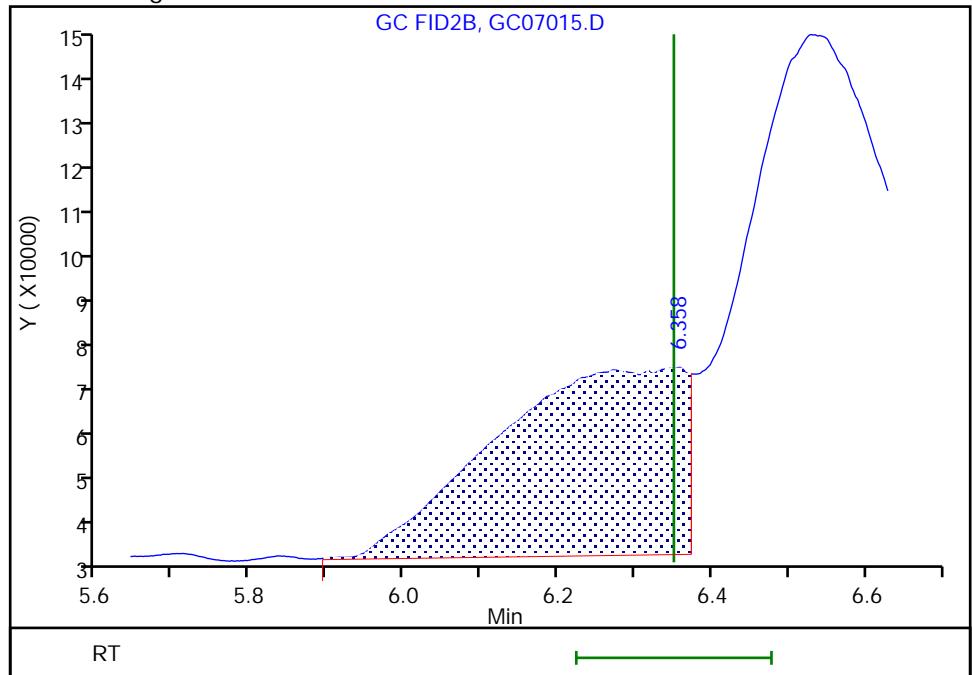

Reviewer: SWK1, 08-Mar-2023 10:48:27
Audit Action: Manually Integrated

Audit Reason: Baseline Smoothing
Page 60 of 134

Eurofins Savannah
Target Compound Quantitation Report

Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07016.D
 Lims ID: icis g4
 Client ID:
 Sample Type: ICIS Calib Level: 4
 Inject. Date: 07-Mar-2023 18:46:59 ALS Bottle#: 0 Worklist Smp#: 8
 Injection Vol: 1.0 ul Dil. Factor: 1.0000
 Sample Info: 680-0084239-008
 Operator ID: Instrument ID: CVGG2
 Sublist: chrom-8015_GLY_VGG*sub2
 Method: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\8015_GLY_VGG.m
 Limit Group: 8015C_DAI
 Last Update: 08-Mar-2023 10:54:47 Calib Date: 07-Mar-2023 19:57:23
 Integrator: Falcon
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07019.D
 Column 1 : J&W DB WAX (0.45 mm) Det: GC FID2B
 Process Host: CTX1619

First Level Reviewer: SWK1 Date: 08-Mar-2023 10:48:37

RT (min.)	Exp RT (min.)	Dlt RT (min.)	Response	Cal Amt ug/ml	OnCol Amt ug/ml	Flags
--------------	------------------	------------------	----------	------------------	--------------------	-------

1 Ethanol, 2-propoxy	2.906	2.906	0.000	1374756	20.0	15.7
2 4-Hydroxy-4-methyl-2-pentanone	3.464	3.464	0.000	1317670	20.0	16.1
3 2-Butoxyethanol	3.753	3.753	0.000	1495618	20.0	14.9
* 4 n-Heptyl Alcohol	4.203	4.203	0.000	7374106	50.0	50.0
5 Dipropylene Glycol Methyl Ether	5.137	5.137	0.000	100988	20.0	16.0
6 Propylene glycol	6.351	6.351	0.000	322840	20.0	14.3 M
7 Ethylene glycol	6.540	6.540	0.000	909818	20.0	15.5
8 2-(2-Butoxyethoxy)ethanol	8.411	8.411	0.000	1097217	20.0	15.1
9 2,2'-Oxybisethanol	9.601	9.601	0.000	507176	20.0	13.4
10 Triethylene Glycol	10.627	10.627	0.000	504087	20.0	13.6
11 Tetraethylene Glycol	11.762	11.762	0.000	1016596	40.0	27.4

QC Flag Legend
Processing Flags

Review Flags

M - Manually Integrated

Reagents:

SG_Gly_CAL_00048

Amount Added: 10.00

Units: uL

SG_GLY_ISTD_00106

Amount Added: 10.00

Units: uL

Run Reagent

Eurofins Savannah

Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07016.D

Injection Date: 07-Mar-2023 18:46:59

Instrument ID: CVGG2

Operator ID:

Lims ID: icis g4

Worklist Smp#: 8

Client ID:

Injection Vol: 1.0 ul


Dil. Factor: 1.0000

ALS Bottle#: 0

Method: 8015_GLY_VGG

Limit Group: 8015C_DAI

Column: J&W DB WAX (0.45 mm)

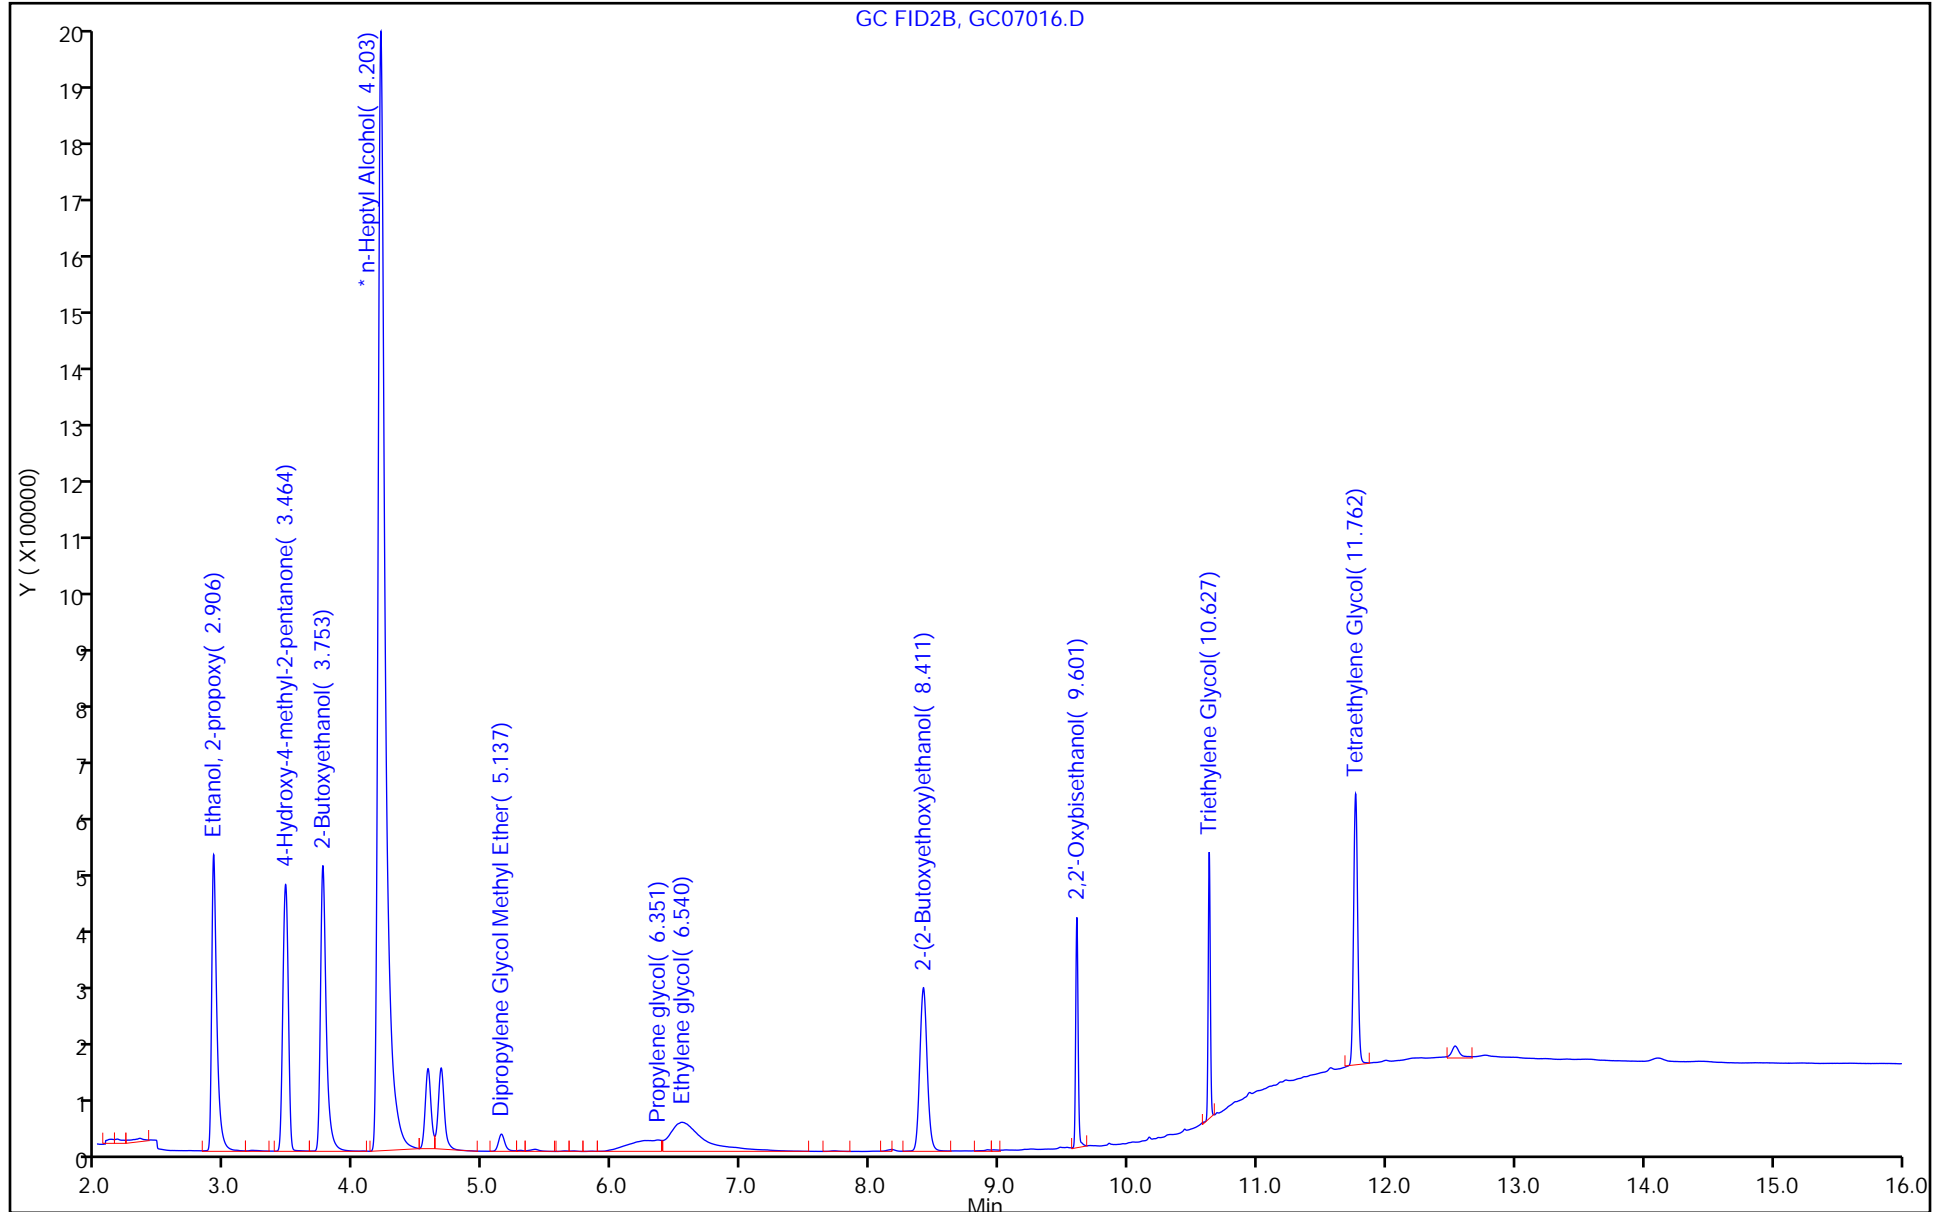

Eurofins Savannah


Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07016.D
Injection Date: 07-Mar-2023 18:46:59 Instrument ID: CVGG2
Lims ID: icis g4
Client ID:
Operator ID: ALS Bottle#: 0 Worklist Smp#: 8
Injection Vol: 1.0 ul Dil. Factor: 1.0000
Method: 8015_GLY_VGG Limit Group: 8015C_DAI
Column: J&W DB WAX (0.45 mm) Detector: GC FID2B

6 Propylene glycol, CAS: 57-55-6

Signal: 1


RT: 6.35
Area: 90286
Amount: 8.044988
Amount Units: ug/ml

Processing Integration Results

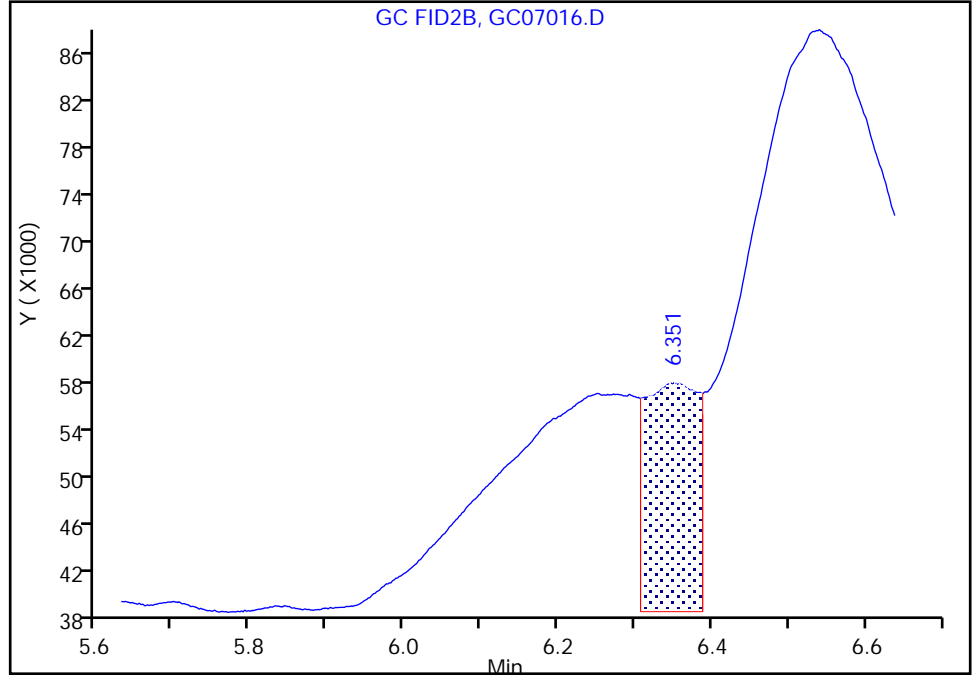

RT: 6.35
Area: 322840
Amount: 14.331117
Amount Units: ug/ml

Manual Integration Results

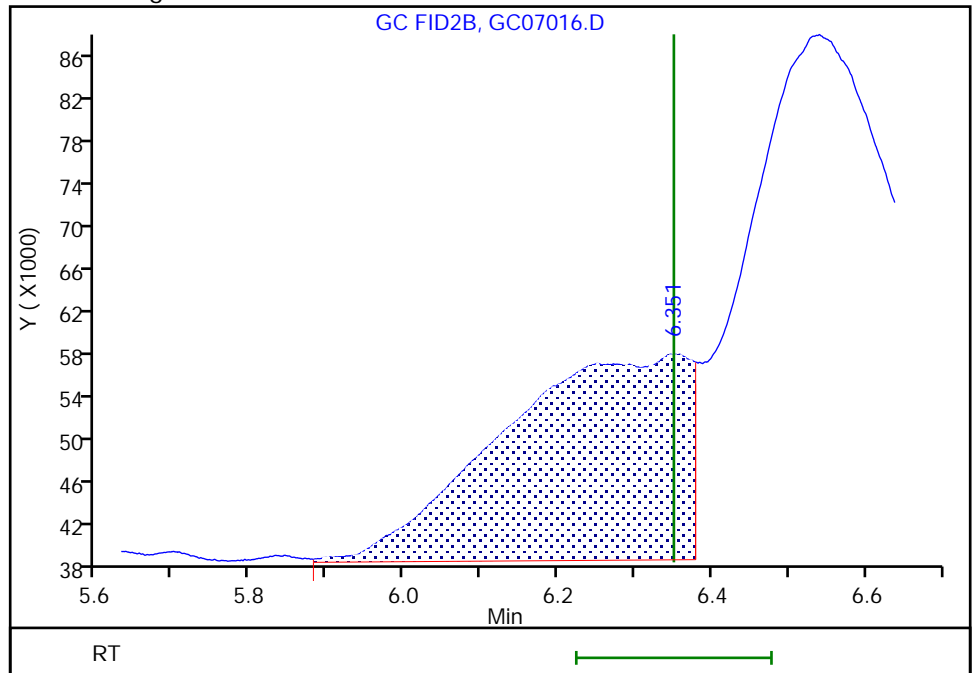

Reviewer: SWK1, 08-Mar-2023 10:48:35
Audit Action: Manually Integrated

Audit Reason: Baseline Smoothing
Page 64 of 134

Eurofins Savannah
Target Compound Quantitation Report

Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07017.D
 Lims ID: ic g3
 Client ID:
 Sample Type: IC Calib Level: 3
 Inject. Date: 07-Mar-2023 19:10:25 ALS Bottle#: 0 Worklist Smp#: 9
 Injection Vol: 1.0 ul Dil. Factor: 1.0000
 Sample Info: 680-0084239-009
 Operator ID: Instrument ID: CVGG2
 Sublist: chrom-8015_GLY_VGG*sub2
 Method: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\8015_GLY_VGG.m
 Limit Group: 8015C_DAI
 Last Update: 08-Mar-2023 10:54:48 Calib Date: 07-Mar-2023 19:57:23
 Integrator: Falcon
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07019.D
 Column 1 : J&W DB WAX (0.45 mm) Det: GC FID2B
 Process Host: CTX1619

First Level Reviewer: SWK1 Date: 08-Mar-2023 10:49:06

RT (min.)	Exp RT (min.)	Dlt RT (min.)	Response	Cal Amt ug/ml	OnCol Amt ug/ml	Flags
1 Ethanol, 2-propoxy						
2.903	2.906	-0.003	777408	10.0	9.96	
2 4-Hydroxy-4-methyl-2-pentanone						
3.458	3.464	-0.006	710717	10.0	9.53	
3 2-Butoxyethanol						
3.753	3.753	0.000	872287	10.0	9.90	
* 4 n-Heptyl Alcohol						
4.207	4.203	0.004	6055528	50.0	50.0	
5 Dipropylene Glycol Methyl Ether						
5.134	5.137	-0.003	53581	10.0	9.50	
6 Propylene glycol						
6.357	6.351	0.006	218465	10.0	11.5	Ma
7 Ethylene glycol						
6.544	6.540	0.004	638794	10.0	13.1	M
8 2-(2-Butoxyethoxy)ethanol						
8.408	8.411	-0.003	632720	10.0	9.85	
9 2,2'-Oxybisethanol						
9.601	9.601	0.000	364788	10.0	11.6	
10 Triethylene Glycol						
10.627	10.627	0.000	366556	10.0	11.8	
11 Tetraethylene Glycol						
11.762	11.762	0.000	735490	20.0	23.9	

QC Flag Legend
Processing Flags

Review Flags

M - Manually Integrated

a - User Assigned ID

Reagents:

SG_Gly_CAL_00048

Amount Added: 5.00

Units: uL

SG_GLY_ISTD_00106

Amount Added: 10.00

Units: uL

Run Reagent

Eurofins Savannah

Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07017.D

Injection Date: 07-Mar-2023 19:10:25

Instrument ID: CVGG2

Operator ID:

Lims ID: ic g3

Worklist Smp#: 9

Client ID:

Injection Vol: 1.0 ul


Dil. Factor: 1.0000

ALS Bottle#: 0

Method: 8015_GLY_VGG

Limit Group: 8015C_DAI

Column: J&W DB WAX (0.45 mm)

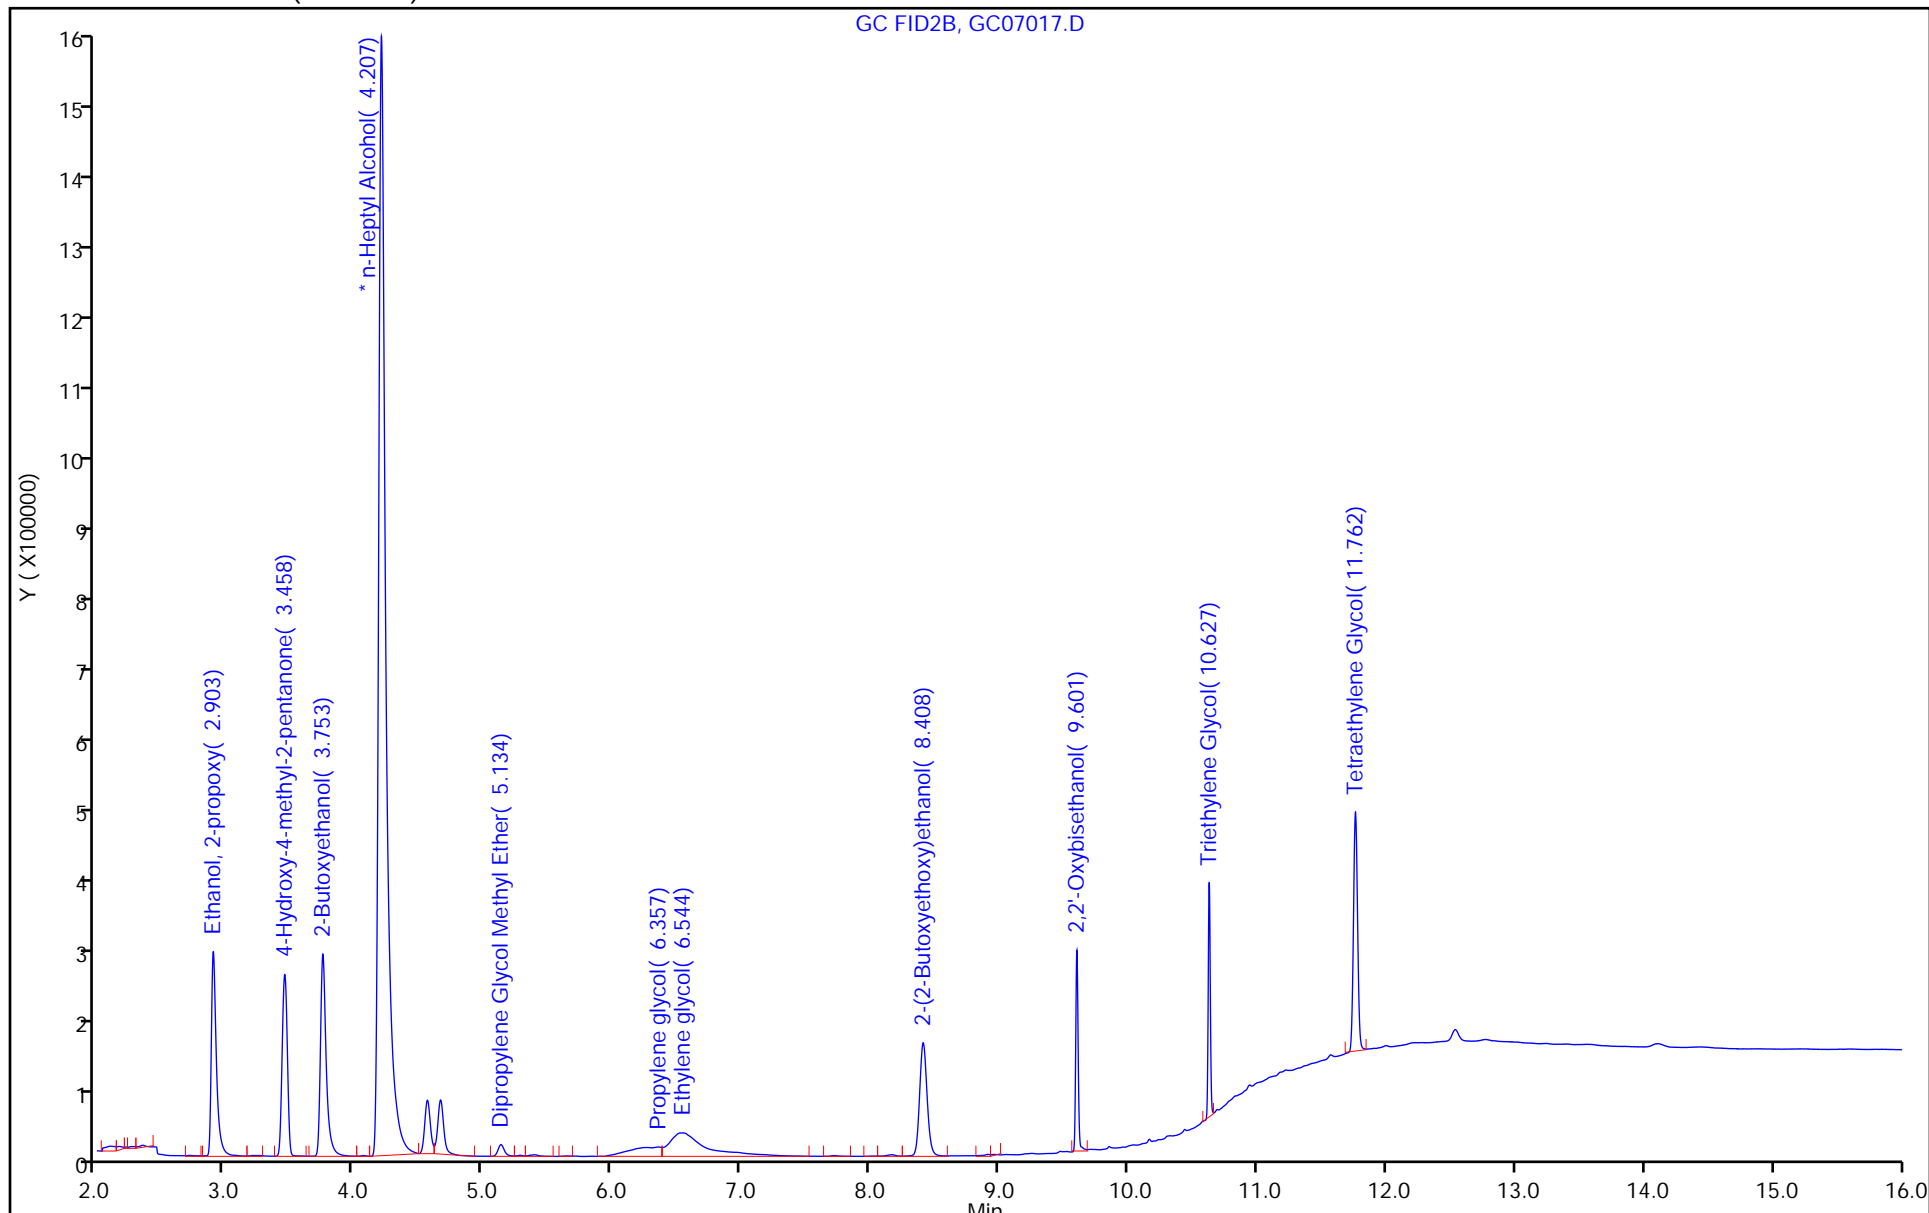

Eurofins Savannah


Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07017.D
Injection Date: 07-Mar-2023 19:10:25 Instrument ID: CVGG2
Lims ID: ic g3
Client ID:
Operator ID: ALS Bottle#: 0 Worklist Smp#: 9
Injection Vol: 1.0 ul Dil. Factor: 1.0000
Method: 8015_GLY_VGG Limit Group: 8015C_DAI
Column: J&W DB WAX (0.45 mm) Detector: GC FID2B

6 Propylene glycol, CAS: 57-55-6

Signal: 1


RT: 6.36
Area: 2479
Amount: 0.234311
Amount Units: ug/ml

Processing Integration Results

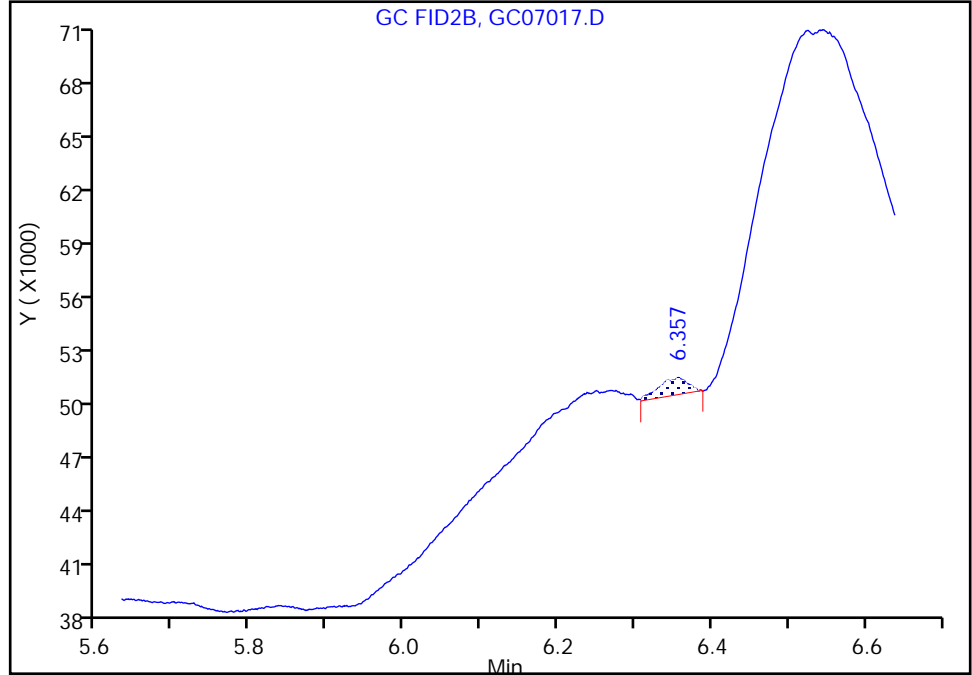

RT: 6.36
Area: 218465
Amount: 11.485503
Amount Units: ug/ml

Manual Integration Results

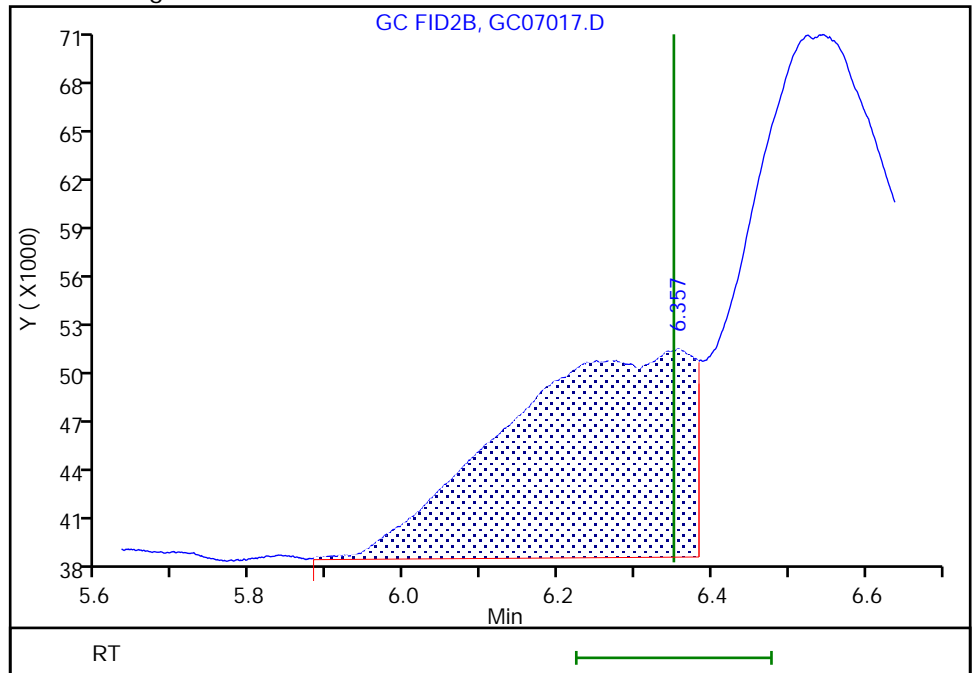

Reviewer: SWK1, 08-Mar-2023 10:49:04

Audit Action: Manually Integrated/Assigned Compound ID Audit Reason: Baseline Smoothing

Eurofins Savannah


Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07017.D
Injection Date: 07-Mar-2023 19:10:25 Instrument ID: CVGG2
Lims ID: ic g3
Client ID:
Operator ID: ALS Bottle#: 0 Worklist Smp#: 9
Injection Vol: 1.0 ul Dil. Factor: 1.0000
Method: 8015_GLY_VGG Limit Group: 8015C_DAI
Column: J&W DB WAX (0.45 mm) Detector: GC FID2B

7 Ethylene glycol, CAS: 107-21-1

Signal: 1


RT: 6.54
Area: 61114
Amount: 1.651632
Amount Units: ug/ml

Processing Integration Results

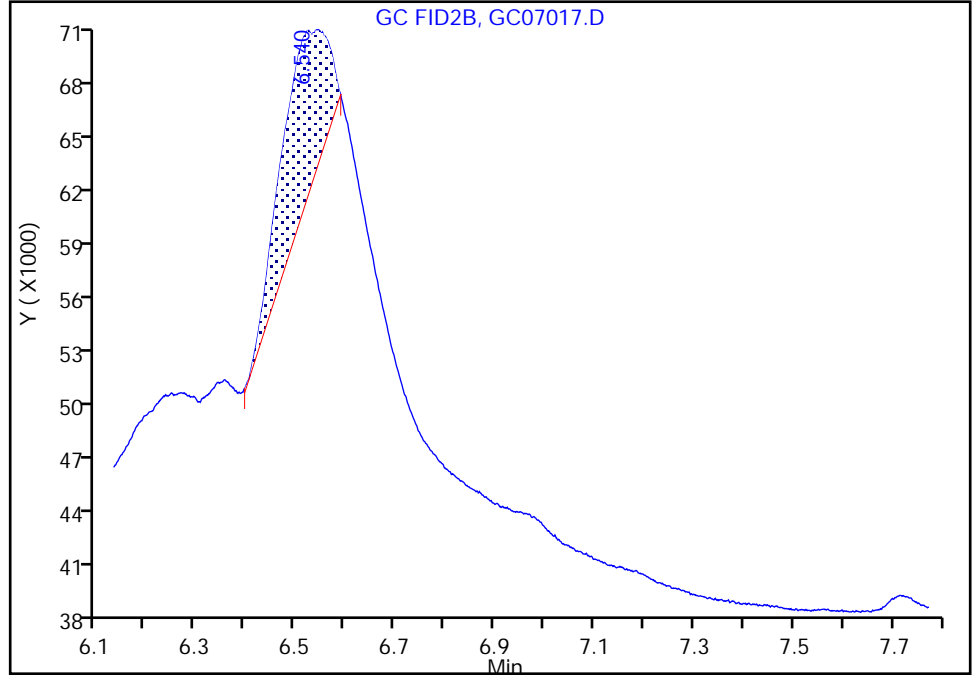

RT: 6.54
Area: 638794
Amount: 13.127941
Amount Units: ug/ml

Manual Integration Results

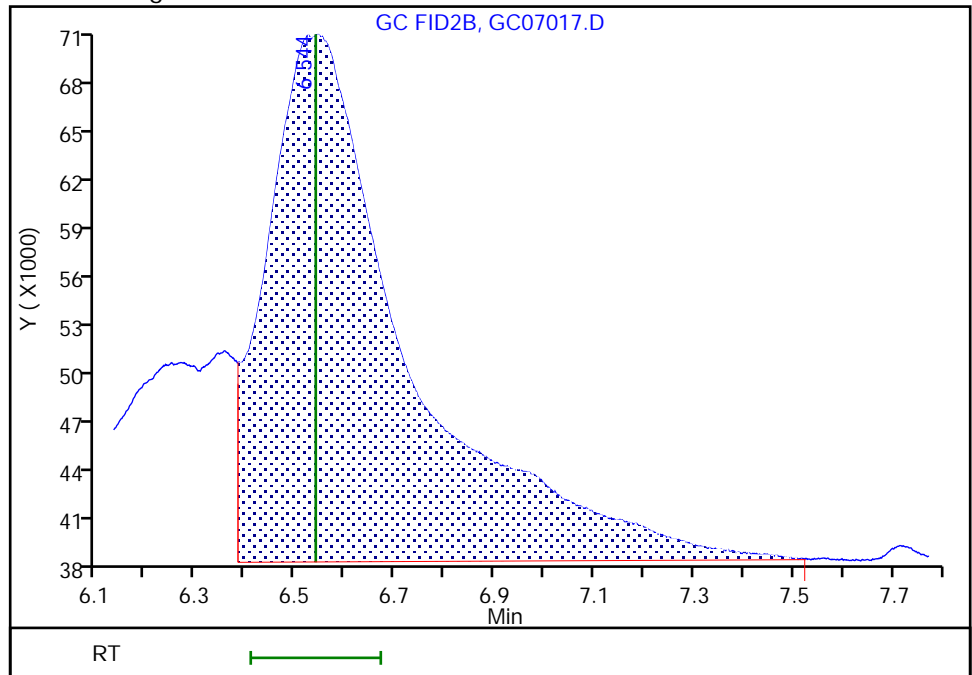

Reviewer: SWK1, 08-Mar-2023 10:49:01
Audit Action: Split an Integrated Peak

Audit Reason: Baseline Smoothing

Eurofins Savannah
Target Compound Quantitation Report

Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07018.D
 Lims ID: ic g2
 Client ID:
 Sample Type: IC Calib Level: 2
 Inject. Date: 07-Mar-2023 19:33:52 ALS Bottle#: 0 Worklist Smp#: 10
 Injection Vol: 1.0 ul Dil. Factor: 1.0000
 Sample Info: 680-0084239-010
 Operator ID: Instrument ID: CVGG2
 Sublist: chrom-8015_GLY_VGG*sub2
 Method: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\8015_GLY_VGG.m
 Limit Group: 8015C_DAI
 Last Update: 08-Mar-2023 10:54:49 Calib Date: 07-Mar-2023 19:57:23
 Integrator: Falcon
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07019.D
 Column 1 : J&W DB WAX (0.45 mm) Det: GC FID2B
 Process Host: CTX1619

First Level Reviewer: SWK1 Date: 08-Mar-2023 10:49:46

RT (min.)	Exp RT (min.)	Dlt RT (min.)	Response	Cal Amt ug/ml	OnCol Amt ug/ml	Flags
1 Ethanol, 2-propoxy						
2.908	2.906	0.002	460254	5.00	5.71	
2 4-Hydroxy-4-methyl-2-pentanone						
3.470	3.464	0.006	452575	5.00	6.00	
3 2-Butoxyethanol						
3.754	3.753	0.001	499197	5.00	5.58	
* 4 n-Heptyl Alcohol						
4.200	4.203	-0.003	5373013	50.0	50.0	
5 Dipropylene Glycol Methyl Ether						
5.141	5.137	0.004	32612	5.00	5.76	
6 Propylene glycol						
6.367	6.351	0.016	90003	5.00	4.35	M
7 Ethylene glycol						
6.538	6.540	-0.002	199343	5.00	4.08	M
8 2-(2-Butoxyethoxy)ethanol						
8.408	8.411	-0.003	362653	5.00	5.45	
9 2,2'-Oxybisethanol						
9.601	9.601	0.000	112793	5.00	3.11	
10 Triethylene Glycol						
10.628	10.627	0.001	115060	5.00	3.05	
11 Tetraethylene Glycol						
11.763	11.762	0.001	213051	10.0	5.93	

QC Flag Legend
Processing Flags

Review Flags

M - Manually Integrated

Reagents:

SG_Gly_CAL_00048

Amount Added: 2.50

Units: uL

SG_GLY_ISTD_00106

Amount Added: 10.00

Units: uL

Run Reagent

Eurofins Savannah

Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07018.D

Injection Date: 07-Mar-2023 19:33:52

Instrument ID: CVGG2

Operator ID:

Lims ID: ic g2

Worklist Smp#: 10

Client ID:

Injection Vol: 1.0 ul


Dil. Factor: 1.0000

ALS Bottle#: 0

Method: 8015_GLY_VGG

Limit Group: 8015C_DAI

Column: J&W DB WAX (0.45 mm)

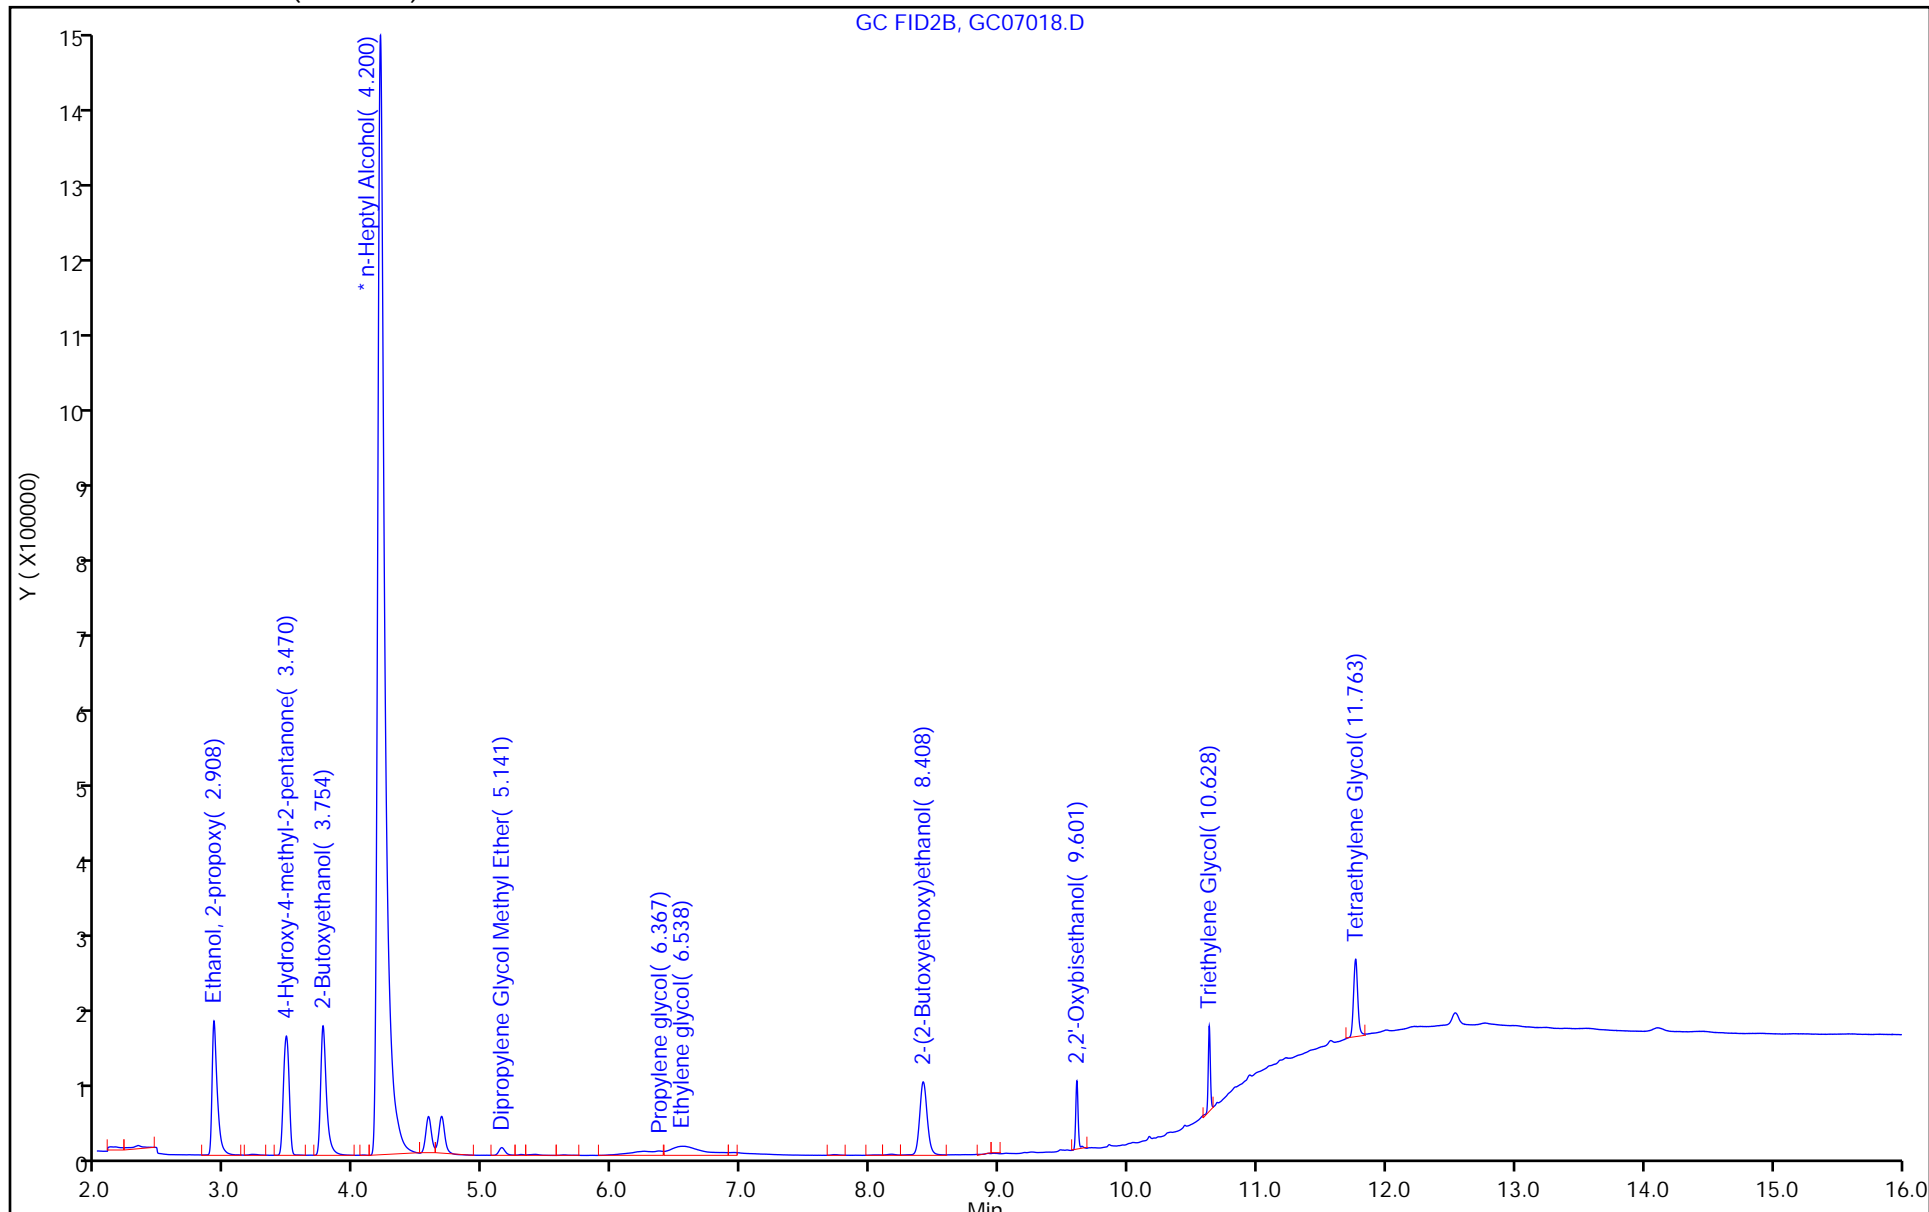

Eurofins Savannah


Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07018.D
Injection Date: 07-Mar-2023 19:33:52 Instrument ID: CVGG2
Lims ID: ic g2
Client ID:
Operator ID: ALS Bottle#: 0 Worklist Smp#: 10
Injection Vol: 1.0 ul Dil. Factor: 1.0000
Method: 8015_GLY_VGG Limit Group: 8015C_DAI
Column: J&W DB WAX (0.45 mm) Detector: GC FID2B

6 Propylene glycol, CAS: 57-55-6

Signal: 1


RT: 6.37
Area: 19149
Amount: 1.579265
Amount Units: ug/ml

Processing Integration Results

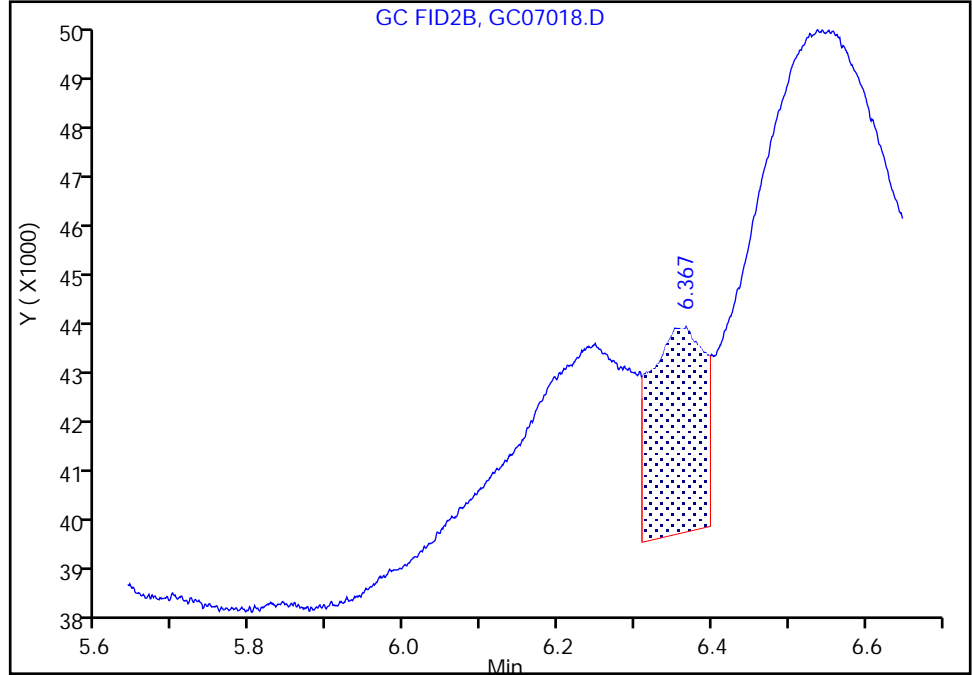

RT: 6.37
Area: 90003
Amount: 4.346405
Amount Units: ug/ml

Manual Integration Results

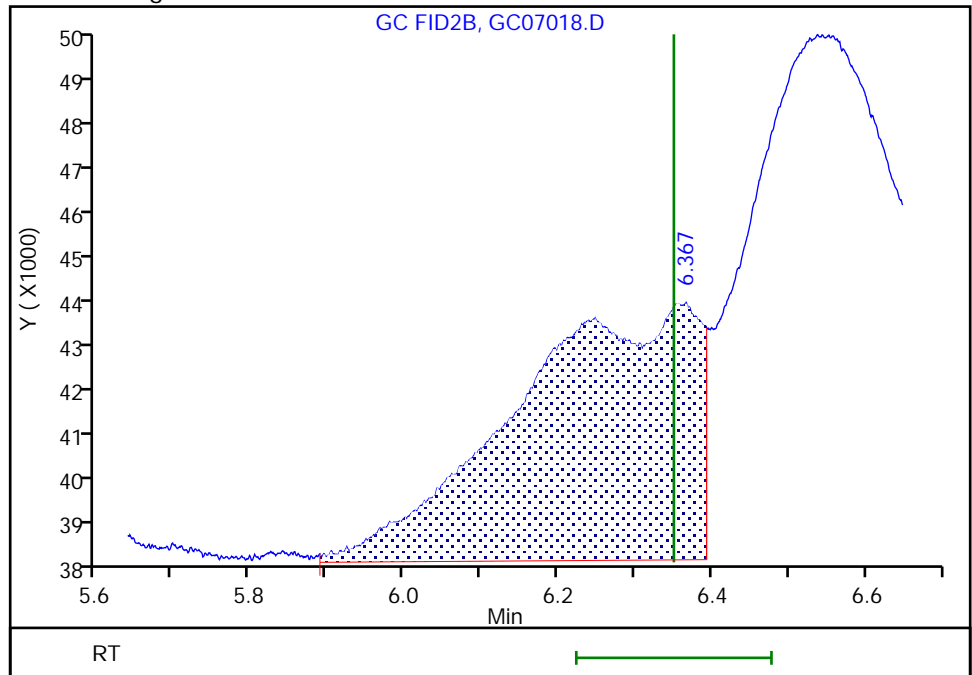

Eurofins Savannah


Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07018.D
Injection Date: 07-Mar-2023 19:33:52 Instrument ID: CVGG2
Lims ID: ic g2
Client ID:
Operator ID: ALS Bottle#: 0 Worklist Smp#: 10
Injection Vol: 1.0 ul Dil. Factor: 1.0000
Method: 8015_GLY_VGG Limit Group: 8015C_DAI
Column: J&W DB WAX (0.45 mm) Detector: GC FID2B

7 Ethylene glycol, CAS: 107-21-1

Signal: 1


RT: 6.54
Area: 128616
Amount: 3.203059
Amount Units: ug/ml

Processing Integration Results

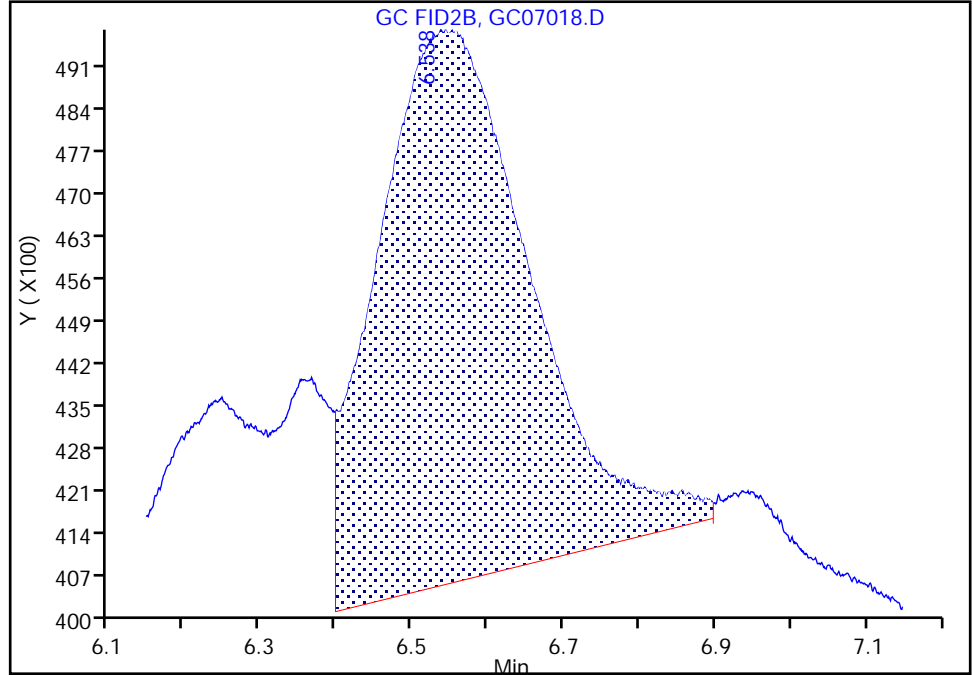

RT: 6.54
Area: 199343
Amount: 4.075566
Amount Units: ug/ml

Manual Integration Results

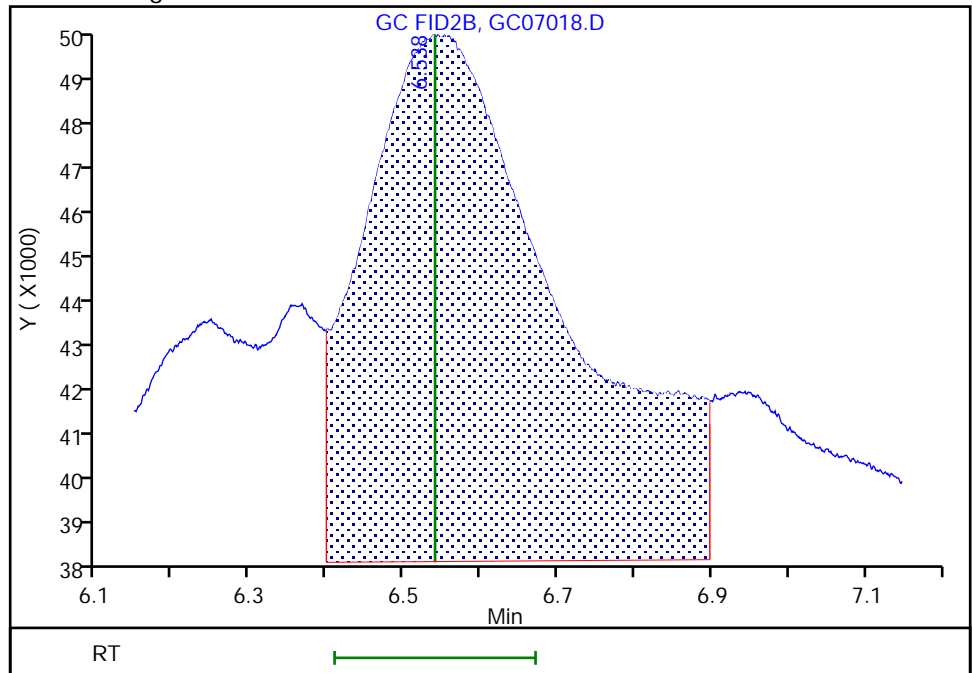

Eurofins Savannah
Target Compound Quantitation Report

Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07019.D
 Lims ID: ic g1
 Client ID:
 Sample Type: IC Calib Level: 1
 Inject. Date: 07-Mar-2023 19:57:23 ALS Bottle#: 0 Worklist Smp#: 11
 Injection Vol: 1.0 ul Dil. Factor: 1.0000
 Sample Info: 680-0084239-011
 Operator ID: Instrument ID: CVGG2
 Sublist: chrom-8015_GLY_VGG*sub2
 Method: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\8015_GLY_VGG.m
 Limit Group: 8015C_DAI
 Last Update: 08-Mar-2023 10:54:50 Calib Date: 07-Mar-2023 19:57:23
 Integrator: Falcon
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07019.D
 Column 1 : J&W DB WAX (0.45 mm) Det: GC FID2B
 Process Host: CTX1619

First Level Reviewer: SWK1 Date: 08-Mar-2023 10:50:04

RT (min.)	Exp RT (min.)	Dlt RT (min.)	Response	Cal Amt ug/ml	OnCol Amt ug/ml	Flags
1 Ethanol, 2-propoxy						
2.907	2.906	0.001	258368	2.00	1.64	
2 4-Hydroxy-4-methyl-2-pentanone						
3.469	3.464	0.005	248723	2.00	1.61	
3 2-Butoxyethanol						
3.755	3.753	0.002	286987	2.00	1.91	
* 4 n-Heptyl Alcohol						
4.200	4.203	-0.003	5788588	50.0	50.0	
5 Dipropylene Glycol Methyl Ether						
5.138	5.137	0.001	17808	2.00	1.73	
6 Propylene glycol						
6.366	6.351	0.015	59431	2.00	1.95	M
7 Ethylene glycol						
6.546	6.540	0.006	114413	2.00	1.78	
8 2-(2-Butoxyethoxy)ethanol						
8.410	8.411	-0.001	220174	2.00	1.94	
9 2,2'-Oxybisethanol						
9.601	9.601	0.000	102548	2.00	2.40	
10 Triethylene Glycol						
10.628	10.627	0.001	107241	2.00	2.41	
11 Tetraethylene Glycol						
11.762	11.762	0.000	200864	4.00	4.85	

QC Flag Legend
Processing Flags

Review Flags

M - Manually Integrated

Reagents:

SG_Gly_CAL_00048

Amount Added: 1.00

Units: uL

SG_GLY_ISTD_00106

Amount Added: 10.00

Units: uL

Run Reagent

Eurofins Savannah

Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07019.D

Injection Date: 07-Mar-2023 19:57:23

Instrument ID: CVGG2

Operator ID:

Lims ID: ic g1

Worklist Smp#: 11

Client ID:

Injection Vol: 1.0 ul


Dil. Factor: 1.0000

ALS Bottle#: 0

Method: 8015_GLY_VGG

Limit Group: 8015C_DAI

Column: J&W DB WAX (0.45 mm)

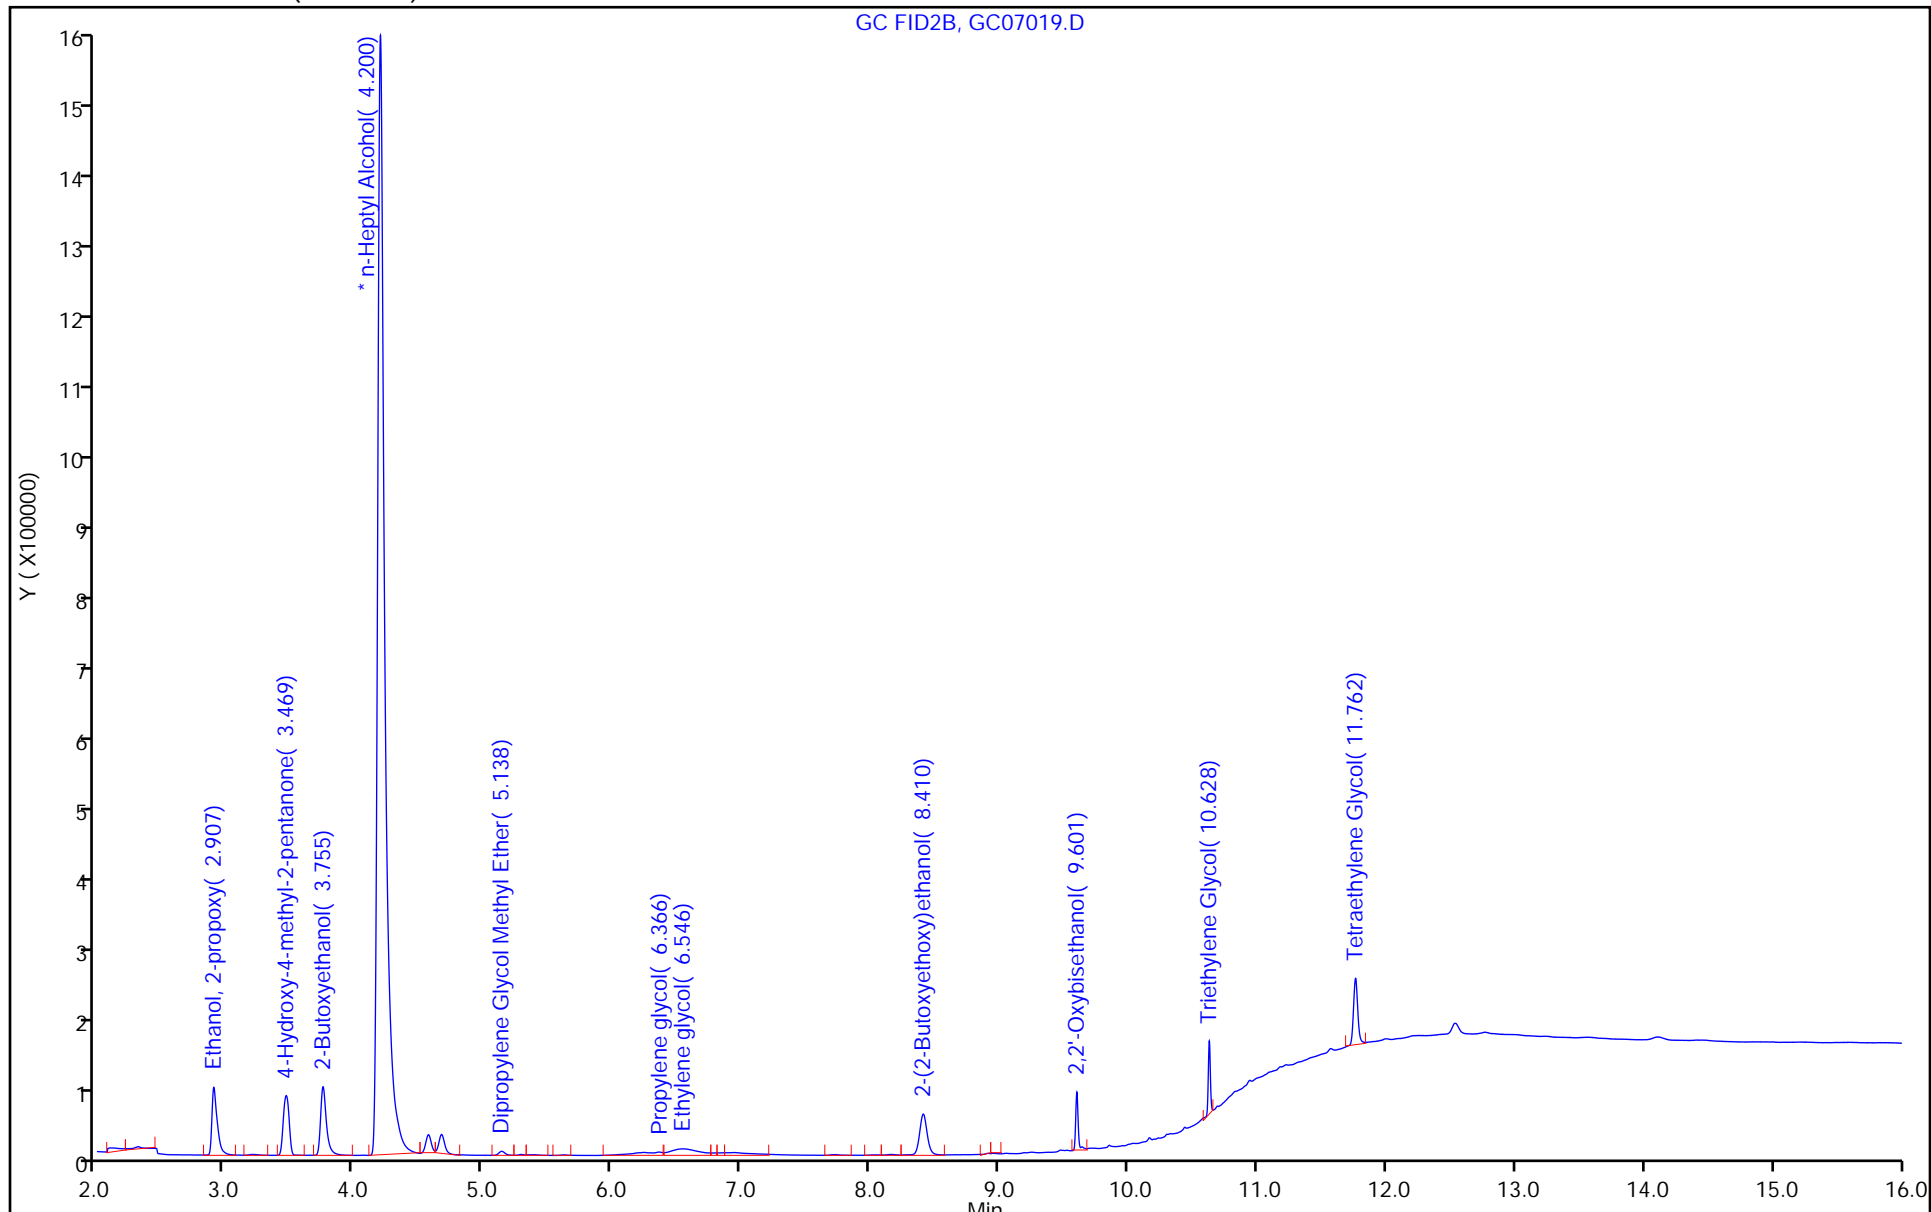

Eurofins Savannah


Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07019.D
Injection Date: 07-Mar-2023 19:57:23 Instrument ID: CVGG2
Lims ID: ic g1
Client ID:
Operator ID: ALS Bottle#: 0 Worklist Smp#: 11
Injection Vol: 1.0 ul Dil. Factor: 1.0000
Method: 8015_GLY_VGG Limit Group: 8015C_DAI
Column: J&W DB WAX (0.45 mm) Detector: GC FID2B

6 Propylene glycol, CAS: 57-55-6

Signal: 1


RT: 6.37
Area: 17958
Amount: 1.178032
Amount Units: ug/ml

Processing Integration Results

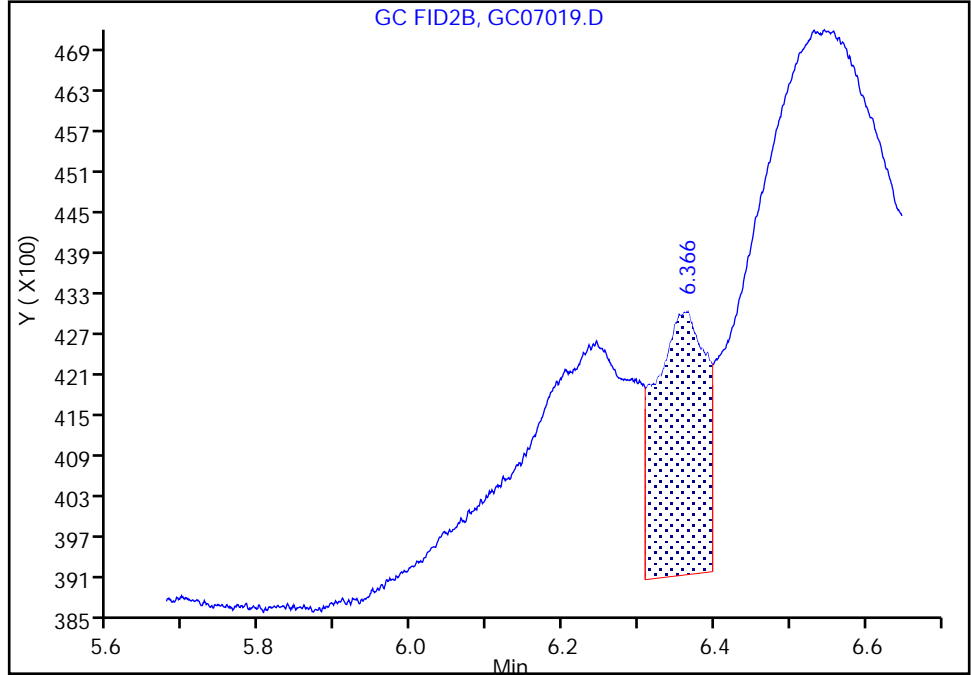

RT: 6.37
Area: 59431
Amount: 1.951189
Amount Units: ug/ml

Manual Integration Results

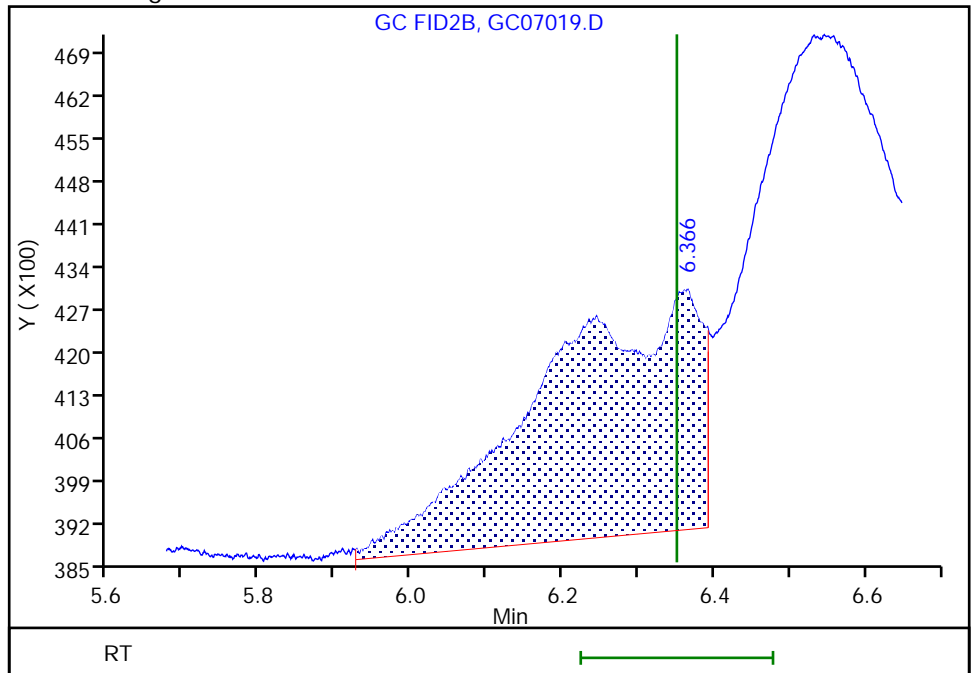

Reviewer: SWK1, 08-Mar-2023 10:49:59
Audit Action: Manually Integrated

Audit Reason: Baseline Smoothing

Calibration


/ Ethanol, 2-propoxy

Curve Type: Linear
 Weighting: Conc
 Origin: None
 Dependency: Response
 Calib Mode: ISTD
 Response Base: AREA
 RF Rounding: 0

Curve Coefficients	
Intercept:	1.408
Slope:	0.503

Error Coefficients	
Standard Error:	3380000
Relative Standard Error:	14.6
Correlation Coefficient:	0.999
Coefficient of Determination (Adjusted):	0.994

ID	Level	Concentration	Rel. Resp.	IS Amount	IS Response	RRF	Used
1	IC 680-766428/11	2.0	2.231701	50.0	5788588.0	1.115851	Y
2	IC 680-766428/10	5.0	4.283016	50.0	5373013.0	0.856603	Y
3	IC 680-766428/9	10.0	6.418994	50.0	6055528.0	0.641899	Y
4	ICIS 680-766428/8	20.0	9.32151	50.0	7374106.0	0.466075	N
5	IC 680-766428/7	50.0	28.849825	50.0	4487093.0	0.576997	Y
6	IC 680-766428/6	80.0	44.670627	50.0	5038257.0	0.558383	N
7	IC 680-766428/5	100.0	49.26498	50.0	5247065.0	0.49265	Y

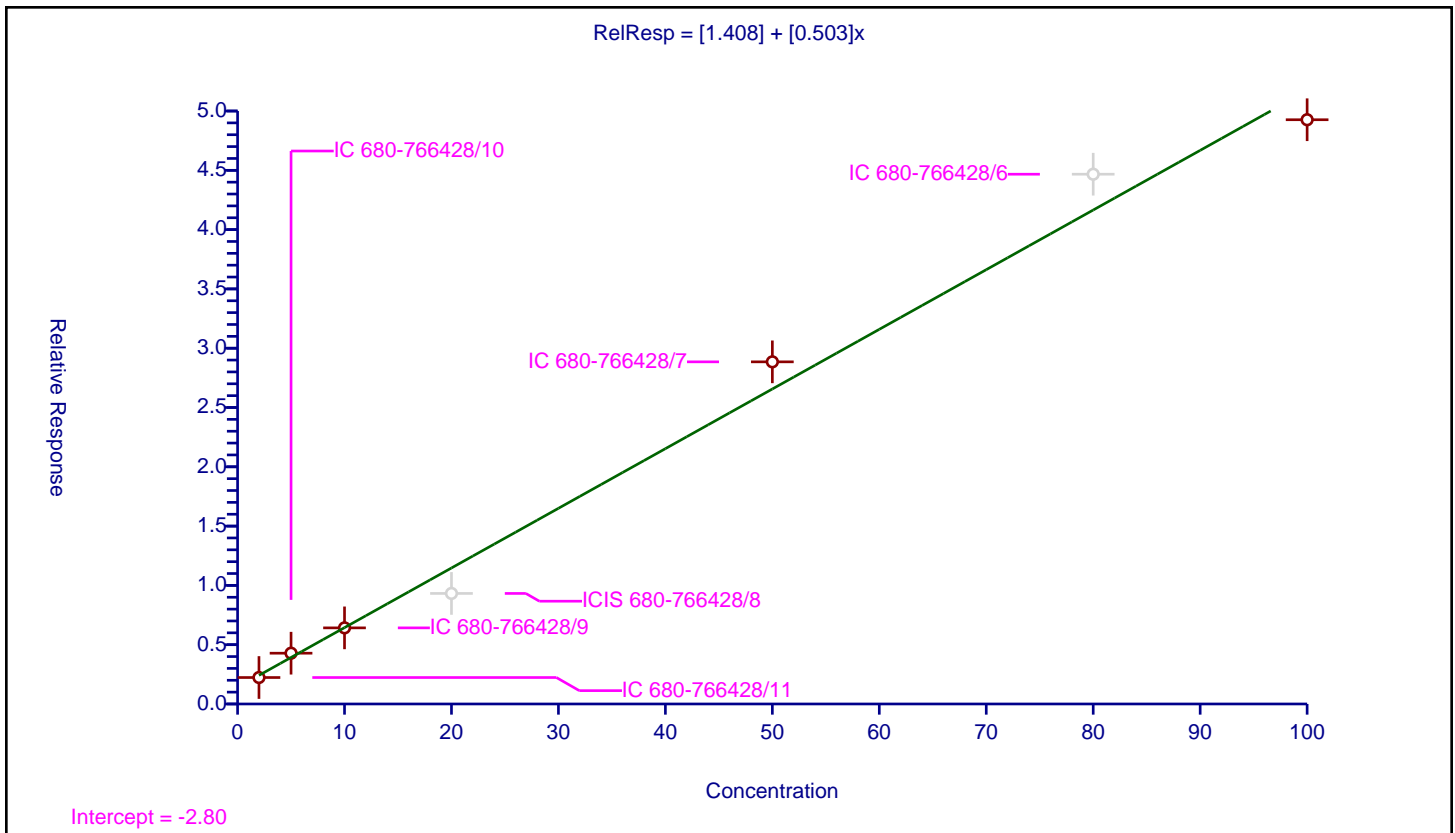

Calibration


/ 4-Hydroxy-4-methyl-2-pentanone

Curve Type: Linear
 Weighting: Conc
 Origin: None
 Dependency: Response
 Calib Mode: ISTD
 Response Base: AREA
 RF Rounding: 0

Curve Coefficients	
Intercept:	1.391
Slope:	0.4699

Error Coefficients	
Standard Error:	3170000
Relative Standard Error:	17.2
Correlation Coefficient:	0.999
Coefficient of Determination (Adjusted):	0.994

ID	Level	Concentration	Rel. Resp.	IS Amount	IS Response	RRF	Used
1	IC 680-766428/11	2.0	2.148391	50.0	5788588.0	1.074195	Y
2	IC 680-766428/10	5.0	4.211557	50.0	5373013.0	0.842311	Y
3	IC 680-766428/9	10.0	5.868332	50.0	6055528.0	0.586833	Y
4	ICIS 680-766428/8	20.0	8.934439	50.0	7374106.0	0.446722	N
5	IC 680-766428/7	50.0	26.833698	50.0	4487093.0	0.536674	Y
6	IC 680-766428/6	80.0	41.808576	50.0	5038257.0	0.522607	N
7	IC 680-766428/5	100.0	46.358621	50.0	5247065.0	0.463586	Y

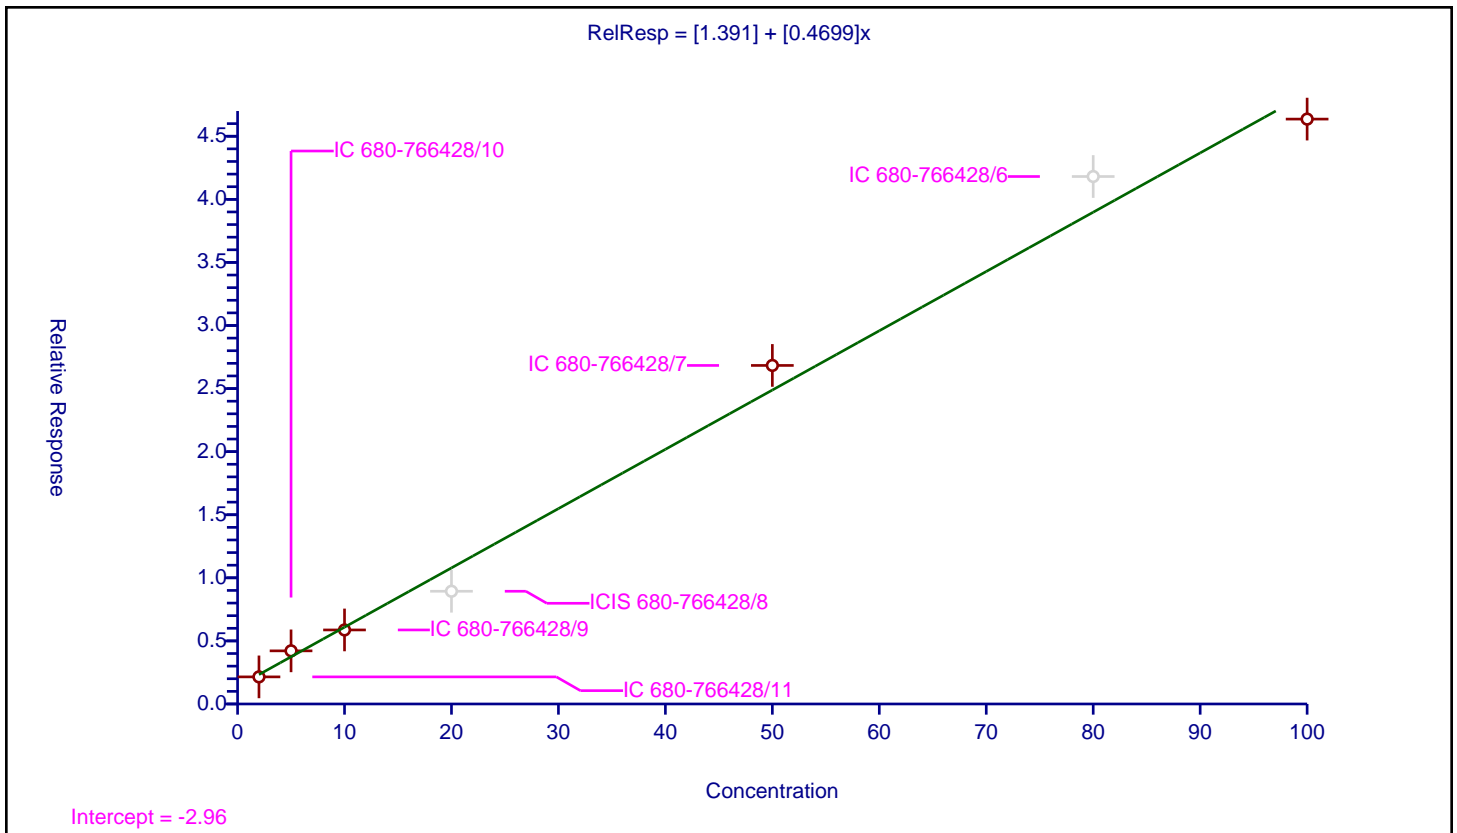

Calibration


/ 2-Butoxyethanol

Curve Type: Linear
 Weighting: Conc_Sq
 Origin: None
 Dependency: Response
 Calib Mode: ISTD
 Response Base: AREA
 RF Rounding: 0

Curve Coefficients	
Intercept:	1.348
Slope:	0.5913

Error Coefficients	
Standard Error:	3760000
Relative Standard Error:	9.3
Correlation Coefficient:	0.999
Coefficient of Determination (Adjusted):	0.991

ID	Level	Concentration	Rel. Resp.	IS Amount	IS Response	RRF	Used
1	IC 680-766428/11	2.0	2.478903	50.0	5788588.0	1.239452	Y
2	IC 680-766428/10	5.0	4.64541	50.0	5373013.0	0.929082	Y
3	IC 680-766428/9	10.0	7.202402	50.0	6055528.0	0.72024	Y
4	ICIS 680-766428/8	20.0	10.141012	50.0	7374106.0	0.507051	N
5	IC 680-766428/7	50.0	31.919876	50.0	4487093.0	0.638398	Y
6	IC 680-766428/6	80.0	48.472696	50.0	5038257.0	0.605909	N
7	IC 680-766428/5	100.0	54.7963	50.0	5247065.0	0.547963	Y

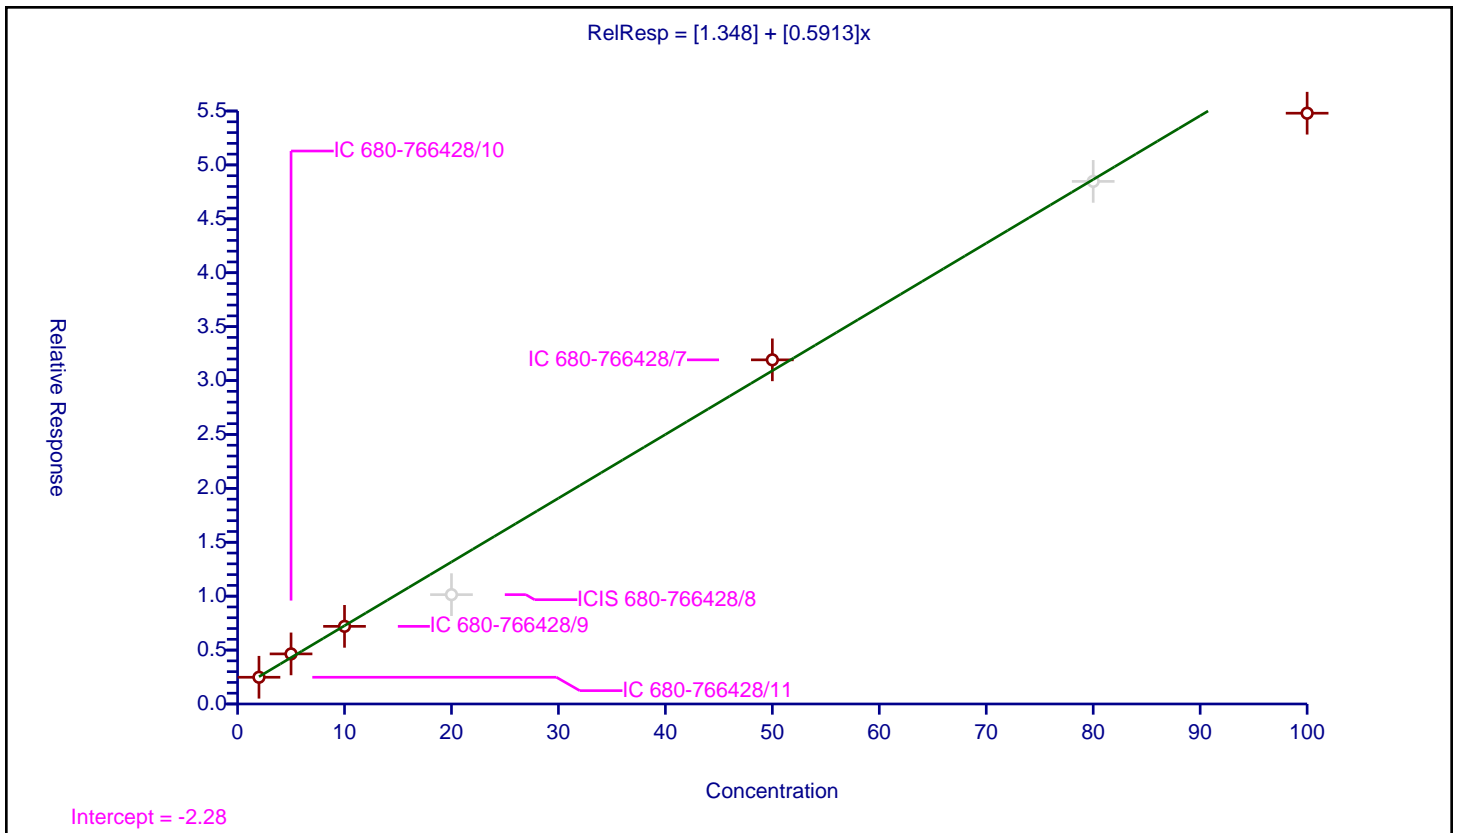

Calibration


/ Dipropylene Glycol Methyl Ether

Curve Type: Linear
 Weighting: Conc
 Origin: None
 Dependency: Response
 Calib Mode: ISTD
 Response Base: AREA
 RF Rounding: 0

Curve Coefficients	
Intercept:	0.08937
Slope:	0.03717

Error Coefficients	
Standard Error:	251000
Relative Standard Error:	12.7
Correlation Coefficient:	0.998
Coefficient of Determination (Adjusted):	0.997

ID	Level	Concentration	Rel. Resp.	IS Amount	IS Response	RRF	Used
1	IC 680-766428/11	2.0	0.15382	50.0	5788588.0	0.07691	Y
2	IC 680-766428/10	5.0	0.30348	50.0	5373013.0	0.060696	Y
3	IC 680-766428/9	10.0	0.442414	50.0	6055528.0	0.044241	Y
4	ICIS 680-766428/8	20.0	0.684747	50.0	7374106.0	0.034237	N
5	IC 680-766428/7	50.0	2.064678	50.0	4487093.0	0.041294	Y
6	IC 680-766428/6	80.0	3.116643	50.0	5038257.0	0.038958	N
7	IC 680-766428/5	100.0	3.69052	50.0	5247065.0	0.036905	Y

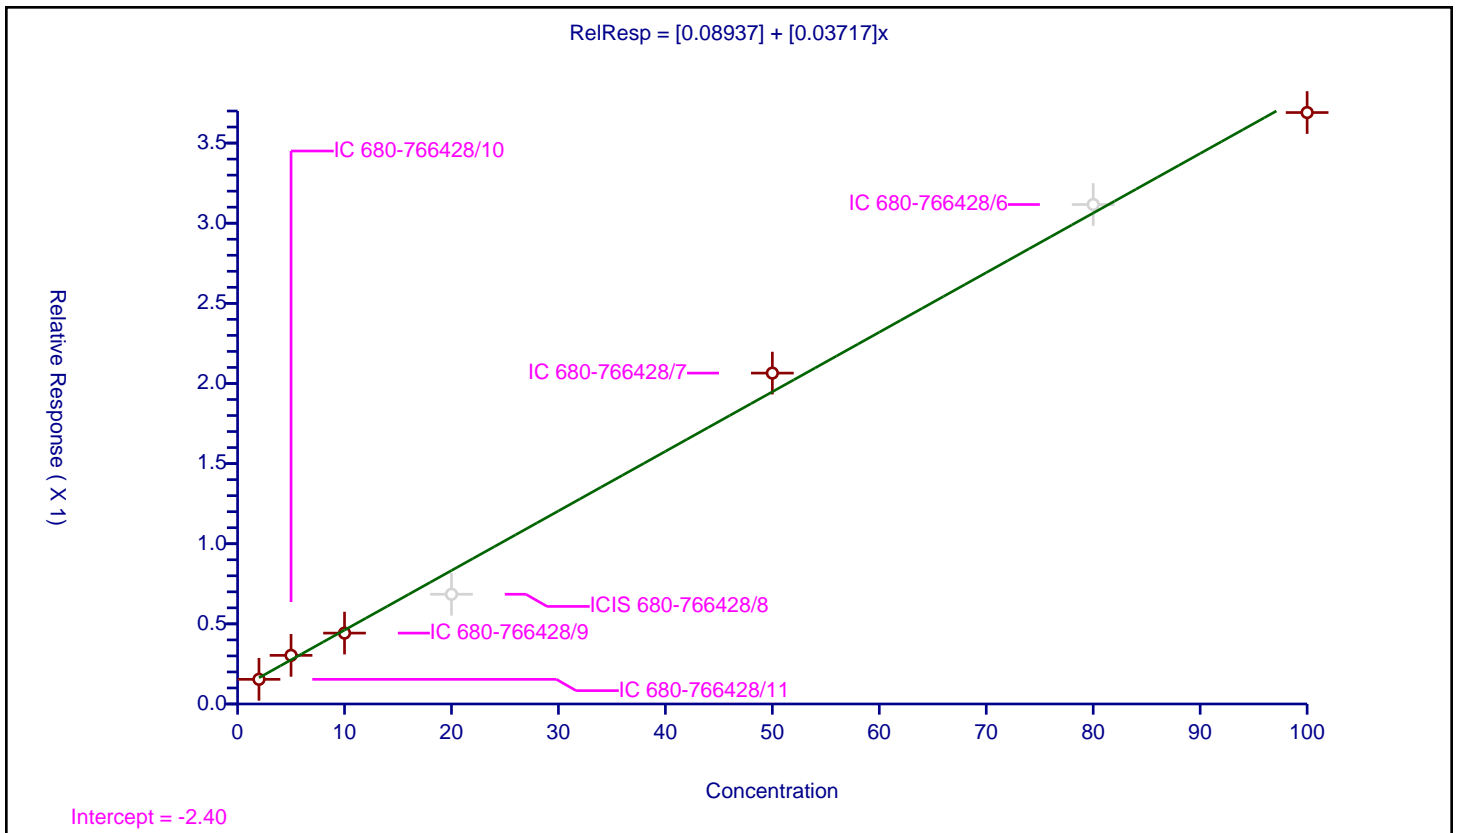

Calibration


/ Propylene glycol

Curve Type: Linear
 Weighting: Conc
 Origin: None
 Dependency: Response
 Calib Mode: ISTD
 Response Base: AREA
 RF Rounding: 0

Curve Coefficients	
Intercept:	0.2492
Slope:	0.1354

Error Coefficients	
Standard Error:	909000
Relative Standard Error:	11.7
Correlation Coefficient:	0.994
Coefficient of Determination (Adjusted):	0.997

ID	Level	Concentration	Rel. Resp.	IS Amount	IS Response	RRF	Used
1	IC 680-766428/11	2.0	0.513346	50.0	5788588.0	0.256673	Y
2	IC 680-766428/10	5.0	0.837547	50.0	5373013.0	0.167509	Y
3	IC 680-766428/9	10.0	1.803848	50.0	6055528.0	0.180385	Y
4	ICIS 680-766428/8	20.0	2.189011	50.0	7374106.0	0.109451	N
5	IC 680-766428/7	50.0	7.211896	50.0	4487093.0	0.144238	Y
6	IC 680-766428/6	80.0	8.618993	50.0	5038257.0	0.107737	N
7	IC 680-766428/5	100.0	13.483605	50.0	5247065.0	0.134836	Y

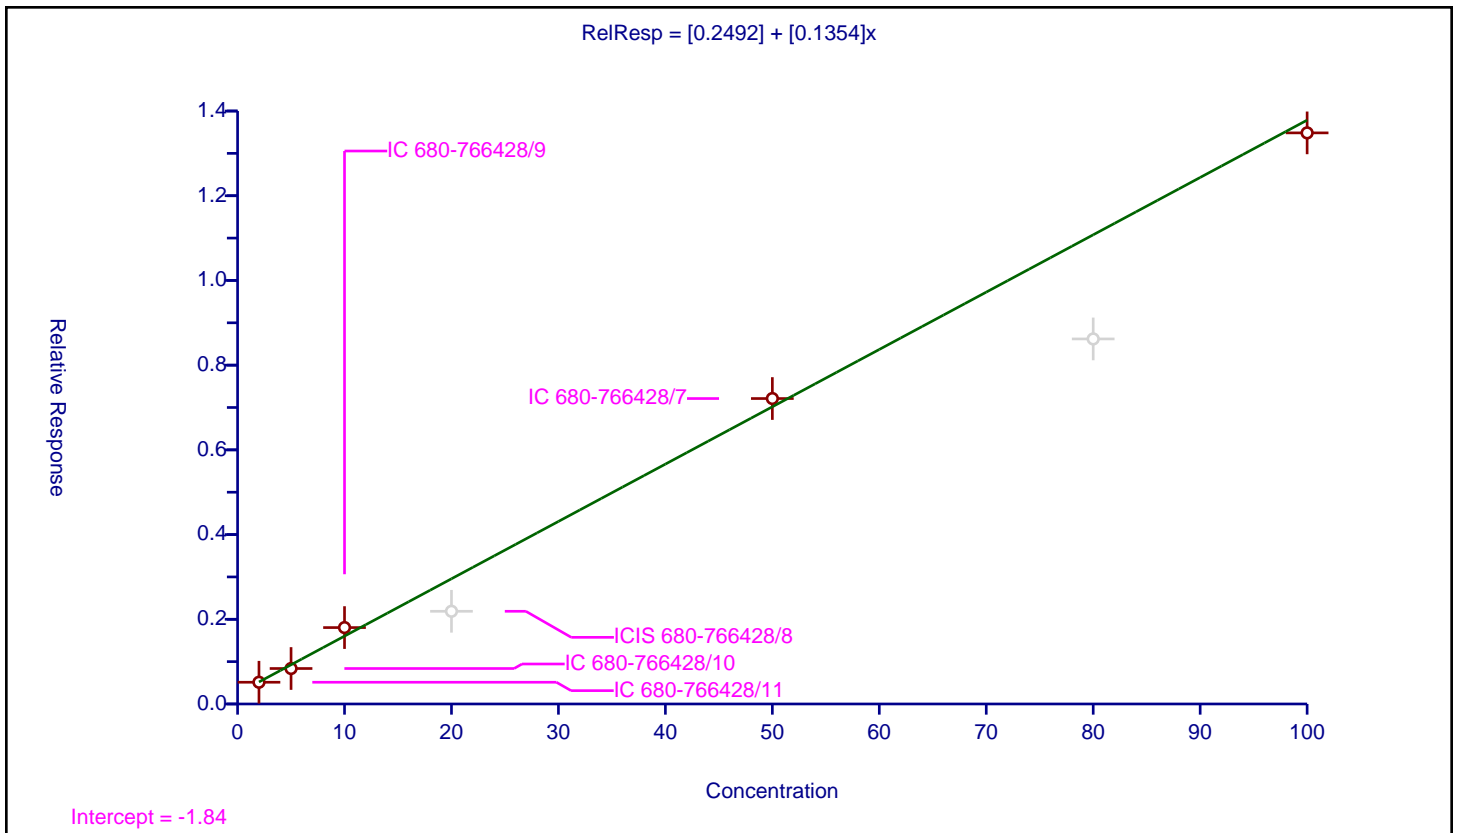

Calibration


/ Ethylene glycol

Curve Type: Linear
 Weighting: Conc
 Origin: None
 Dependency: Response
 Calib Mode: ISTD
 Response Base: AREA
 RF Rounding: 0

Curve Coefficients	
Intercept:	0.3155
Slope:	0.3777

Error Coefficients	
Standard Error:	2500000
Relative Standard Error:	21.9
Correlation Coefficient:	0.990
Coefficient of Determination (Adjusted):	0.991

ID	Level	Concentration	Rel. Resp.	IS Amount	IS Response	RRF	Used
1	IC 680-766428/11	2.0	0.988263	50.0	5788588.0	0.494132	Y
2	IC 680-766428/10	5.0	1.855039	50.0	5373013.0	0.371008	Y
3	IC 680-766428/9	10.0	5.27447	50.0	6055528.0	0.527447	Y
4	ICIS 680-766428/8	20.0	6.169005	50.0	7374106.0	0.30845	N
5	IC 680-766428/7	50.0	19.258237	50.0	4487093.0	0.385165	Y
6	IC 680-766428/6	80.0	23.059641	50.0	5038257.0	0.288246	N
7	IC 680-766428/5	100.0	37.284024	50.0	5247065.0	0.37284	Y

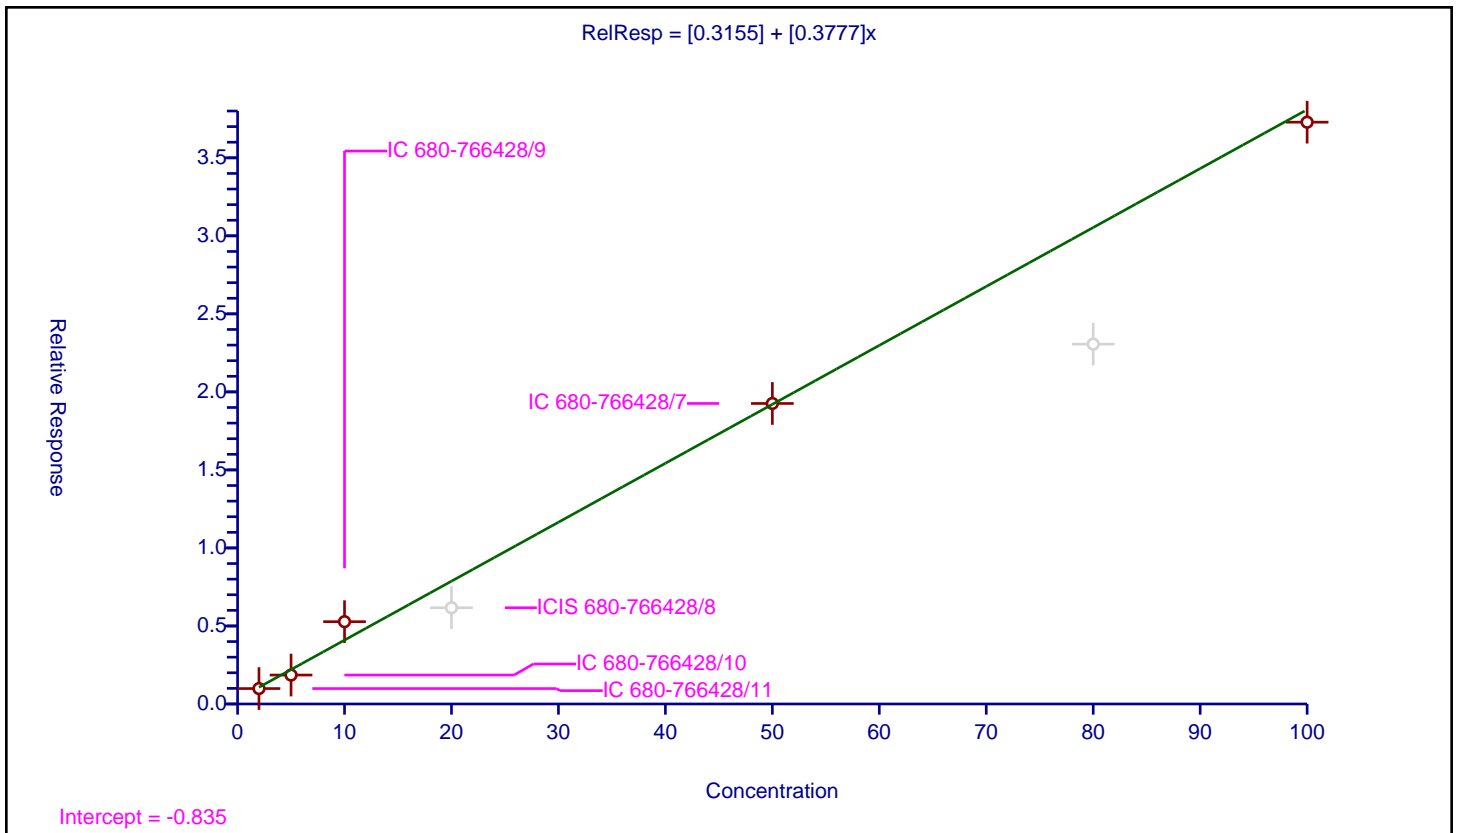

Calibration


/ 2-(2-Butoxyethoxy)ethanol

Curve Type: Linear
 Weighting: Conc_Sq
 Origin: None
 Dependency: Response
 Calib Mode: ISTD
 Response Base: AREA
 RF Rounding: 0

Curve Coefficients	
Intercept:	1.09
Slope:	0.4196

Error Coefficients	
Standard Error:	2740000
Relative Standard Error:	6.8
Correlation Coefficient:	0.997
Coefficient of Determination (Adjusted):	0.995

ID	Level	Concentration	Rel. Resp.	IS Amount	IS Response	RRF	Used
1	IC 680-766428/11	2.0	1.901794	50.0	5788588.0	0.950897	Y
2	IC 680-766428/10	5.0	3.374764	50.0	5373013.0	0.674953	Y
3	IC 680-766428/9	10.0	5.224317	50.0	6055528.0	0.522432	Y
4	ICIS 680-766428/8	20.0	7.439661	50.0	7374106.0	0.371983	N
5	IC 680-766428/7	50.0	22.55009	50.0	4487093.0	0.451002	Y
6	IC 680-766428/6	80.0	32.186359	50.0	5038257.0	0.402329	N
7	IC 680-766428/5	100.0	40.32359	50.0	5247065.0	0.403236	Y

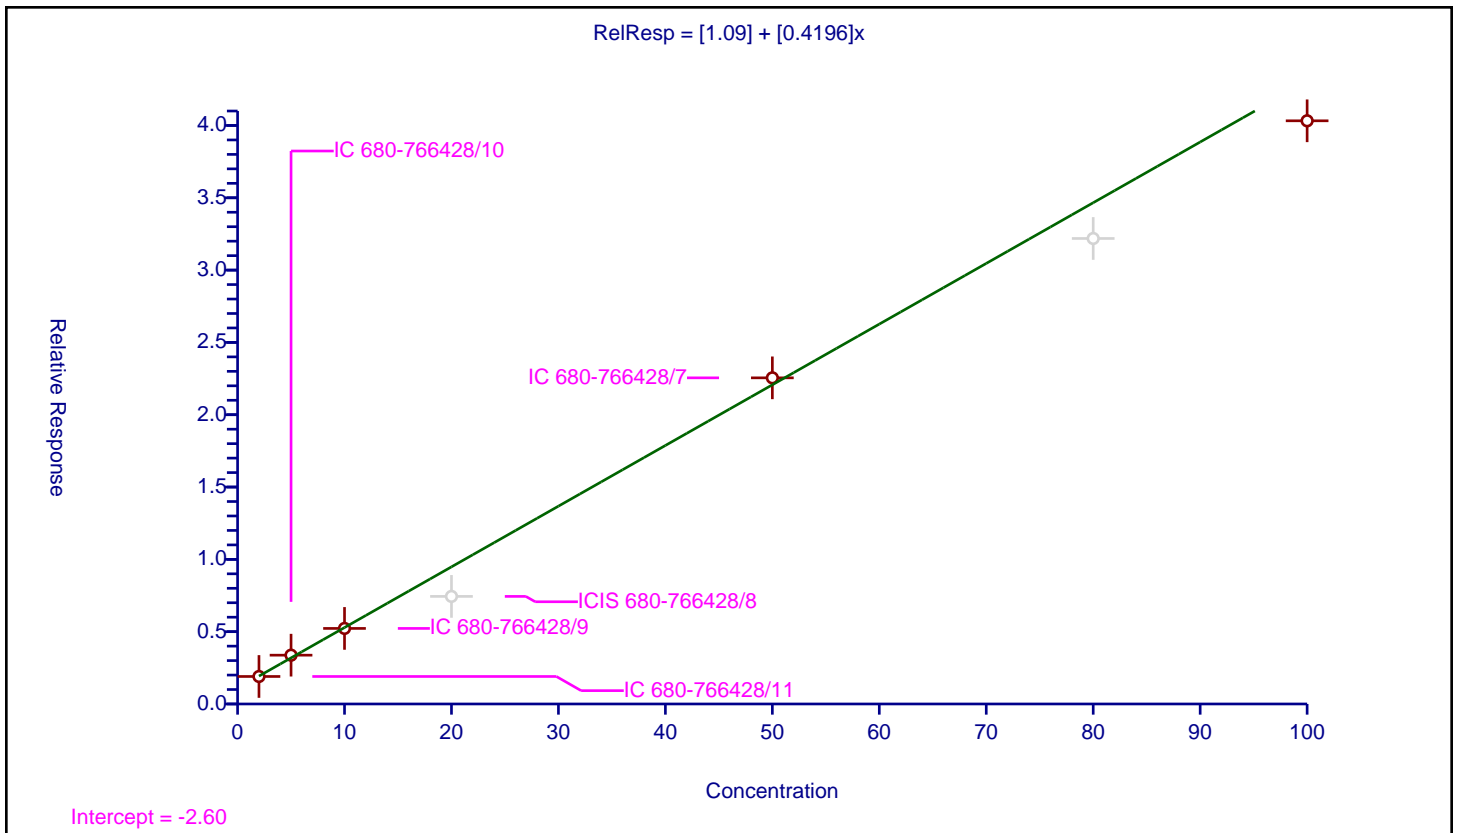

Calibration


/ 2,2'-Oxybisethanol

Curve Type: Linear
 Weighting: Conc
 Origin: None
 Dependency: Response
 Calib Mode: ISTD
 Response Base: AREA
 RF Rounding: 0

Curve Coefficients	
Intercept:	0.329
Slope:	0.2316

Error Coefficients	
Standard Error:	1550000
Relative Standard Error:	26.5
Correlation Coefficient:	0.994
Coefficient of Determination (Adjusted):	0.992

ID	Level	Concentration	Rel. Resp.	IS Amount	IS Response	RRF	Used
1	IC 680-766428/11	2.0	0.885777	50.0	5788588.0	0.442889	Y
2	IC 680-766428/10	5.0	1.049625	50.0	5373013.0	0.209925	Y
3	IC 680-766428/9	10.0	3.012025	50.0	6055528.0	0.301202	Y
4	ICIS 680-766428/8	20.0	3.438898	50.0	7374106.0	0.171945	N
5	IC 680-766428/7	50.0	12.337308	50.0	4487093.0	0.246746	Y
6	IC 680-766428/6	80.0	14.477229	50.0	5038257.0	0.180965	N
7	IC 680-766428/5	100.0	23.039261	50.0	5247065.0	0.230393	Y

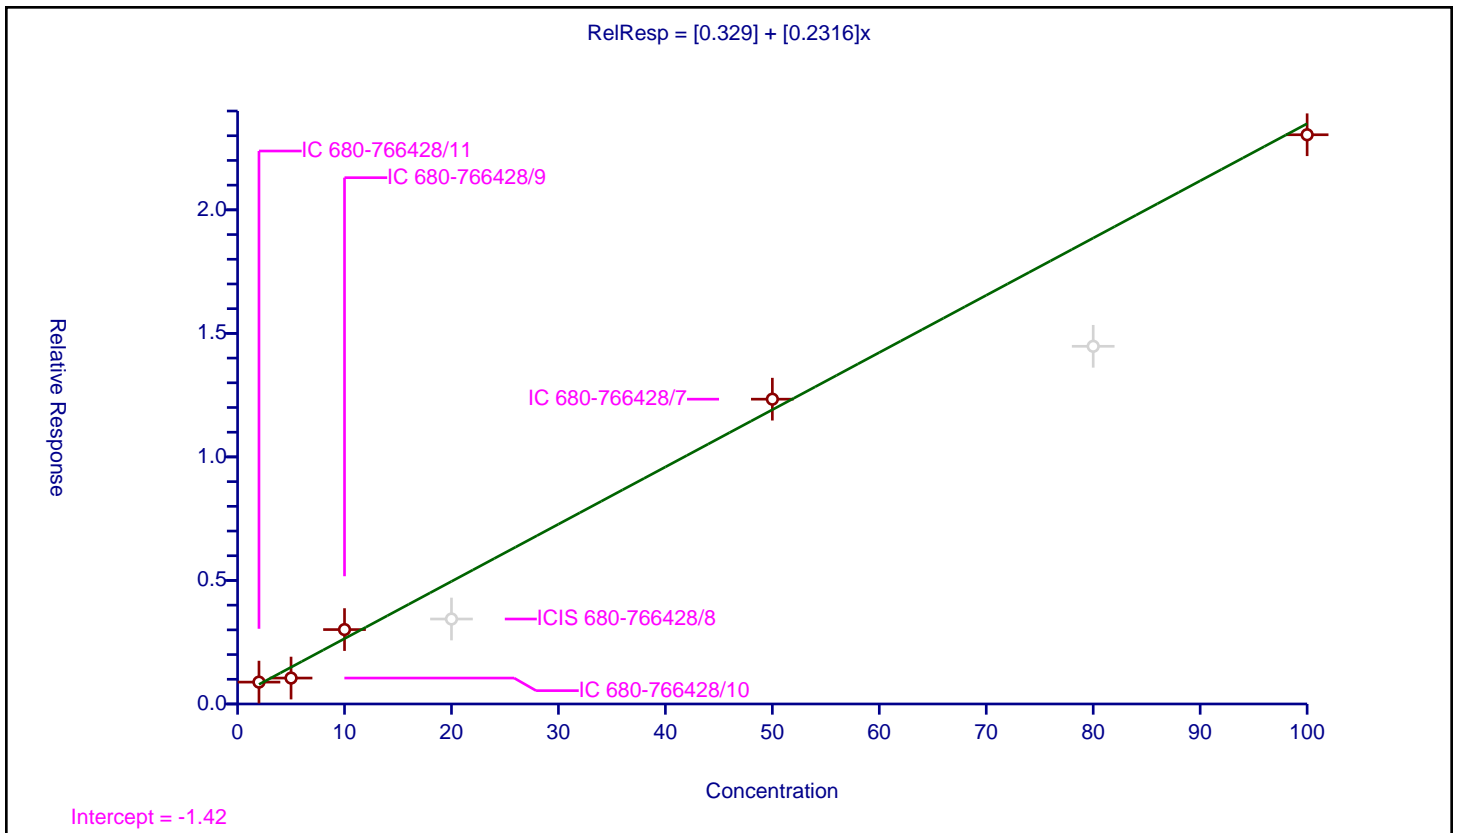

Calibration


/ Triethylene Glycol

Curve Type: Linear
 Weighting: Conc
 Origin: None
 Dependency: Response
 Calib Mode: ISTD
 Response Base: AREA
 RF Rounding: 0

Curve Coefficients	
Intercept:	0.3888
Slope:	0.2234

Error Coefficients	
Standard Error:	1510000
Relative Standard Error:	27.5
Correlation Coefficient:	0.992
Coefficient of Determination (Adjusted):	0.991

ID	Level	Concentration	Rel. Resp.	IS Amount	IS Response	RRF	Used
1	IC 680-766428/11	2.0	0.926314	50.0	5788588.0	0.463157	Y
2	IC 680-766428/10	5.0	1.070721	50.0	5373013.0	0.214144	Y
3	IC 680-766428/9	10.0	3.026623	50.0	6055528.0	0.302662	Y
4	ICIS 680-766428/8	20.0	3.417953	50.0	7374106.0	0.170898	N
5	IC 680-766428/7	50.0	11.729465	50.0	4487093.0	0.234589	Y
6	IC 680-766428/6	80.0	13.904561	50.0	5038257.0	0.173807	N
7	IC 680-766428/5	100.0	22.490659	50.0	5247065.0	0.224907	Y

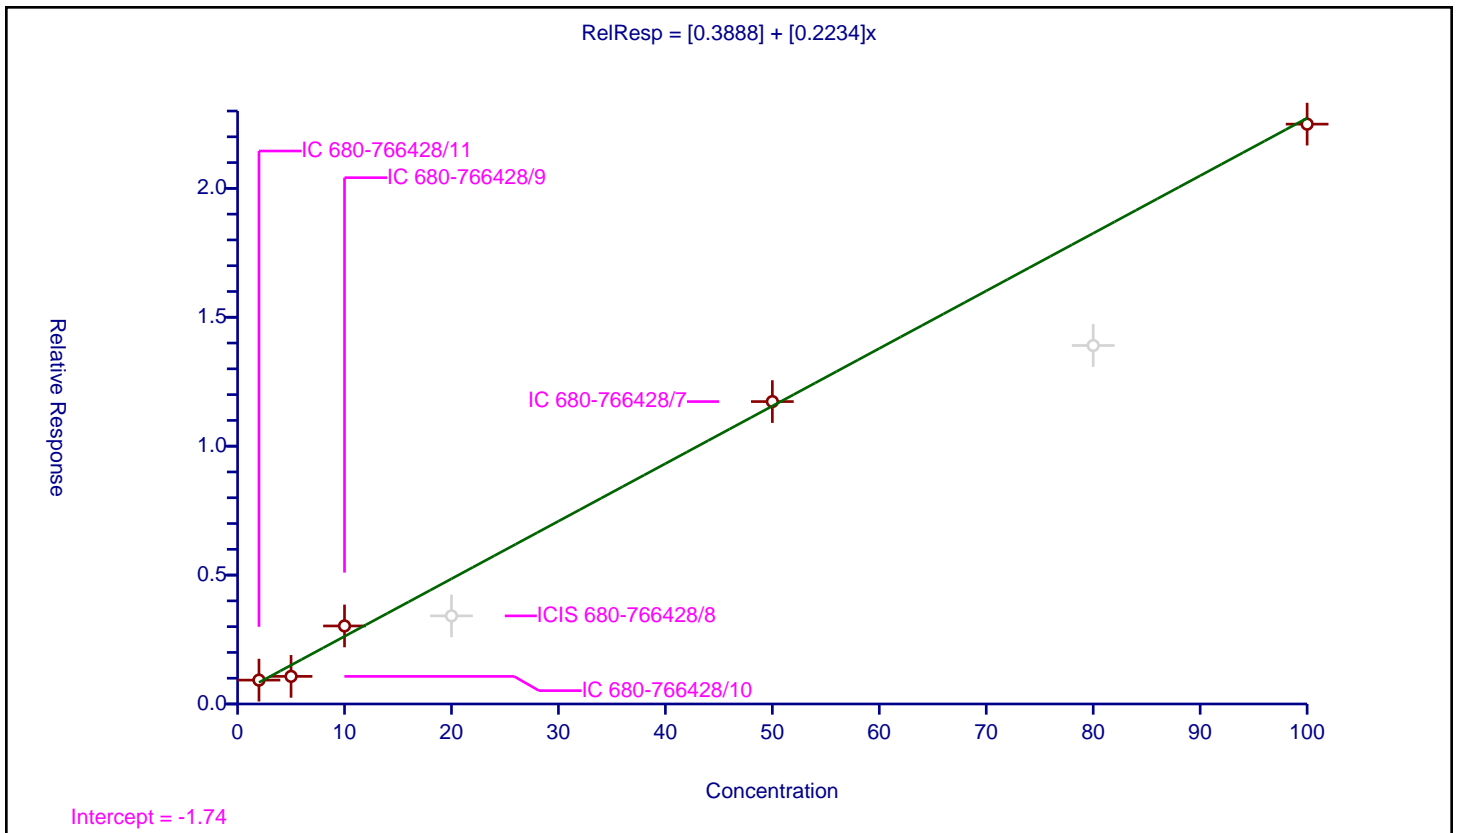

Calibration


/ Tetraethylene Glycol

Curve Type: Linear
 Weighting: Conc
 Origin: None
 Dependency: Response
 Calib Mode: ISTD
 Response Base: AREA
 RF Rounding: 0

Curve Coefficients	
Intercept:	0.6281
Slope:	0.2282

Error Coefficients	
Standard Error:	3070000
Relative Standard Error:	28.7
Correlation Coefficient:	0.991
Coefficient of Determination (Adjusted):	0.991

ID	Level	Concentration	Rel. Resp.	IS Amount	IS Response	RRF	Used
1	IC 680-766428/11	4.0	1.735	50.0	5788588.0	0.43375	Y
2	IC 680-766428/10	10.0	1.982603	50.0	5373013.0	0.19826	Y
3	IC 680-766428/9	20.0	6.072881	50.0	6055528.0	0.303644	Y
4	ICIS 680-766428/8	40.0	6.893012	50.0	7374106.0	0.172325	N
5	IC 680-766428/7	100.0	23.656107	50.0	4487093.0	0.236561	Y
6	IC 680-766428/6	160.0	28.426954	50.0	5038257.0	0.177668	N
7	IC 680-766428/5	200.0	45.923235	50.0	5247065.0	0.229616	Y

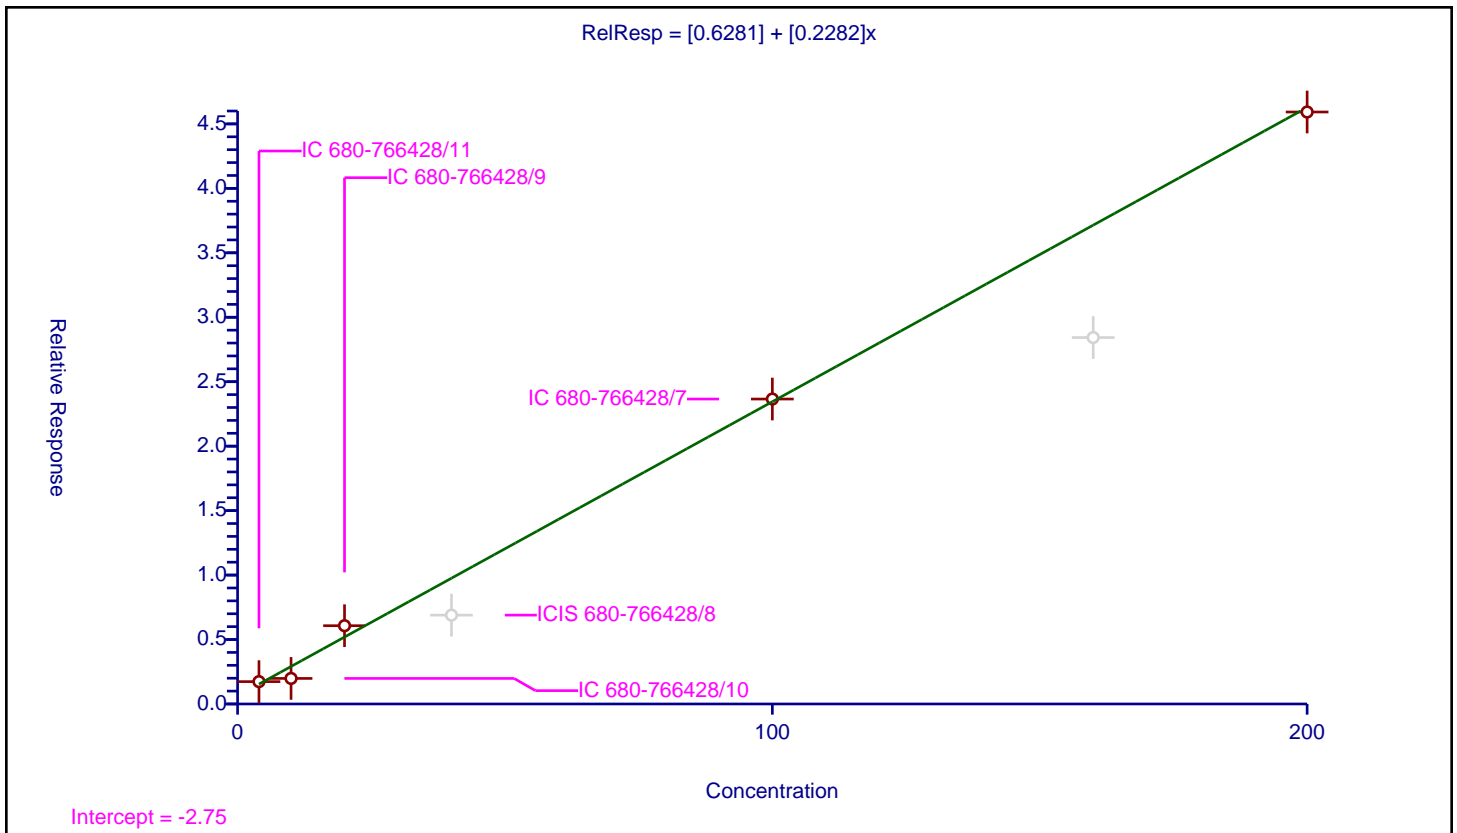

FORM VII
GC SEMI VOA CONTINUING CALIBRATION DATA

Lab Name: Eurofins Savannah Job No.: 580-124266-1
 SDG No.: _____
 Lab Sample ID: ICV 680-766428/12 Calibration Date: 03/07/2023 20:20
 Instrument ID: CVGG2 Calib Start Date: 03/07/2023 17:36
 GC Column: J&W DB WAX ID: 0.45 (mm) Calib End Date: 03/07/2023 19:57
 Lab File ID: GC07020.D Conc. Units: mg/L

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Ethanol, 2-propoxy	Lin1		0.6548		23.2	20.0	16.2	20.0
4-Hydroxy-4-methyl-2-pentano ne	Lin1		0.6118		23.1	20.0	15.4	20.0
2-Butoxyethanol	Lin2		0.7573		23.3	20.0	16.7	20.0
Dipropylene Glycol Methyl Ether	Lin1		0.0454		22.0	20.0	10.1	20.0
Propylene glycol	Lin1		0.1410		19.0	20.0	-5.0	20.0
Ethylene glycol	Lin1		0.4131		21.0	20.0	5.2	20.0
2-(2-Butoxyethoxy)ethanol	Lin2		0.5016		21.3	20.0	6.5	20.0
2,2'-Oxybisethanol	Lin1		0.2301		18.4	20.0	-7.8	20.0
Triethylene Glycol	Lin1		0.2452		20.2	20.0	1.1	20.0
Tetraethylene Glycol	Lin1		0.2448		40.2	40.0	0.4	20.0

FORM VII
GC SEMI VOA CONTINUING CALIBRATION RETENTION TIME SUMMARY

Lab Name: Eurofins Savannah Job No.: 580-124266-1
 SDG No.: _____
 Lab Sample ID: ICV 680-766428/12 Calibration Date: 03/07/2023 20:20
 Instrument ID: CVGG2 Calib Start Date: 03/07/2023 17:36
 GC Column: J&W DB WAX ID: 0.45 (mm) Calib End Date: 03/07/2023 19:57
 Lab File ID: GC07020.D

Analyte	RT	RT WINDOW	
		FROM	TO
Ethanol, 2-propoxy	2.91	2.86	2.97
4-Hydroxy-4-methyl-2-pentanone	3.46	3.40	3.54
2-Butoxyethanol	3.75	3.68	3.83
Dipropylene Glycol Methyl Ether	5.14	5.03	5.24
Propylene glycol	6.35	6.21	6.46
Ethylene glycol	6.53	6.46	6.73
2-(2-Butoxyethoxy)ethanol	8.41	8.24	8.58
2,2'-Oxybisethanol	9.60	9.41	9.80
Triethylene Glycol	10.63	10.42	10.85
Tetraethylene Glycol	11.76	11.55	12.02

Eurofins Savannah
Target Compound Quantitation Report

Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07020.D
 Lims ID: icv gly
 Client ID:
 Sample Type: CCV
 Inject. Date: 07-Mar-2023 20:20:49 ALS Bottle#: 0 Worklist Smp#: 12
 Injection Vol: 1.0 ul Dil. Factor: 1.0000
 Sample Info: 680-0084239-012
 Operator ID: Instrument ID: CVGG2
 Sublist: chrom-8015_GLY_VGG*sub2
 Method: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\8015_GLY_VGG.m
 Limit Group: 8015C_DAI
 Last Update: 08-Mar-2023 11:27:12 Calib Date: 07-Mar-2023 19:57:23
 Integrator: Falcon
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07019.D
 Column 1 : J&W DB WAX (0.45 mm) Det: GC FID2B
 Process Host: CTX1619

First Level Reviewer: SWK1 Date: 08-Mar-2023 10:50:28

RT (min.)	Exp RT (min.)	Dlt RT (min.)	Response	Cal Amt ug/ml	OnCol Amt ug/ml	Flags
1 Ethanol, 2-propoxy						
2.905	2.914	-0.009	1543890	20.0	23.2	
2 4-Hydroxy-4-methyl-2-pentanone						
3.464	3.469	-0.005	1442495	20.0	23.1	
3 2-Butoxyethanol						
3.754	3.758	-0.004	1785640	20.0	23.3	
* 4 n-Heptyl Alcohol						
4.203	4.204	-0.001	5894548	50.0	50.0	
5 Dipropylene Glycol Methyl Ether						
5.135	5.136	-0.001	107047	20.0	22.0	
6 Propylene glycol						
6.354	6.332	0.022	332520	20.0	19.0	M
7 Ethylene glycol						
6.525	6.595	-0.070	973933	20.0	21.0	Ma M
8 2-(2-Butoxyethoxy)ethanol						
8.408	8.407	0.001	1182586	20.0	21.3	
9 2,2'-Oxybisethanol						
9.600	9.604	-0.004	542469	20.0	18.4	
10 Triethylene Glycol						
10.628	10.637	-0.009	578237	20.0	20.2	
11 Tetraethylene Glycol						
11.761	11.789	-0.028	1154545	40.0	40.2	

QC Flag Legend
Processing Flags

Review Flags

M - Manually Integrated

a - User Assigned ID

Reagents:

SG_GlyICV_00055

Amount Added: 10.00

Units: uL

SG_GLY_ISTD_00106

Amount Added: 10.00

Units: uL

Run Reagent

Eurofins Savannah

Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07020.D

Injection Date: 07-Mar-2023 20:20:49

Instrument ID: CVGG2

Operator ID:

Lims ID: icv gly

Worklist Smp#: 12

Client ID:

Injection Vol: 1.0 ul


Dil. Factor: 1.0000

ALS Bottle#: 0

Method: 8015_GLY_VGG

Limit Group: 8015C_DAI

Column: J&W DB WAX (0.45 mm)

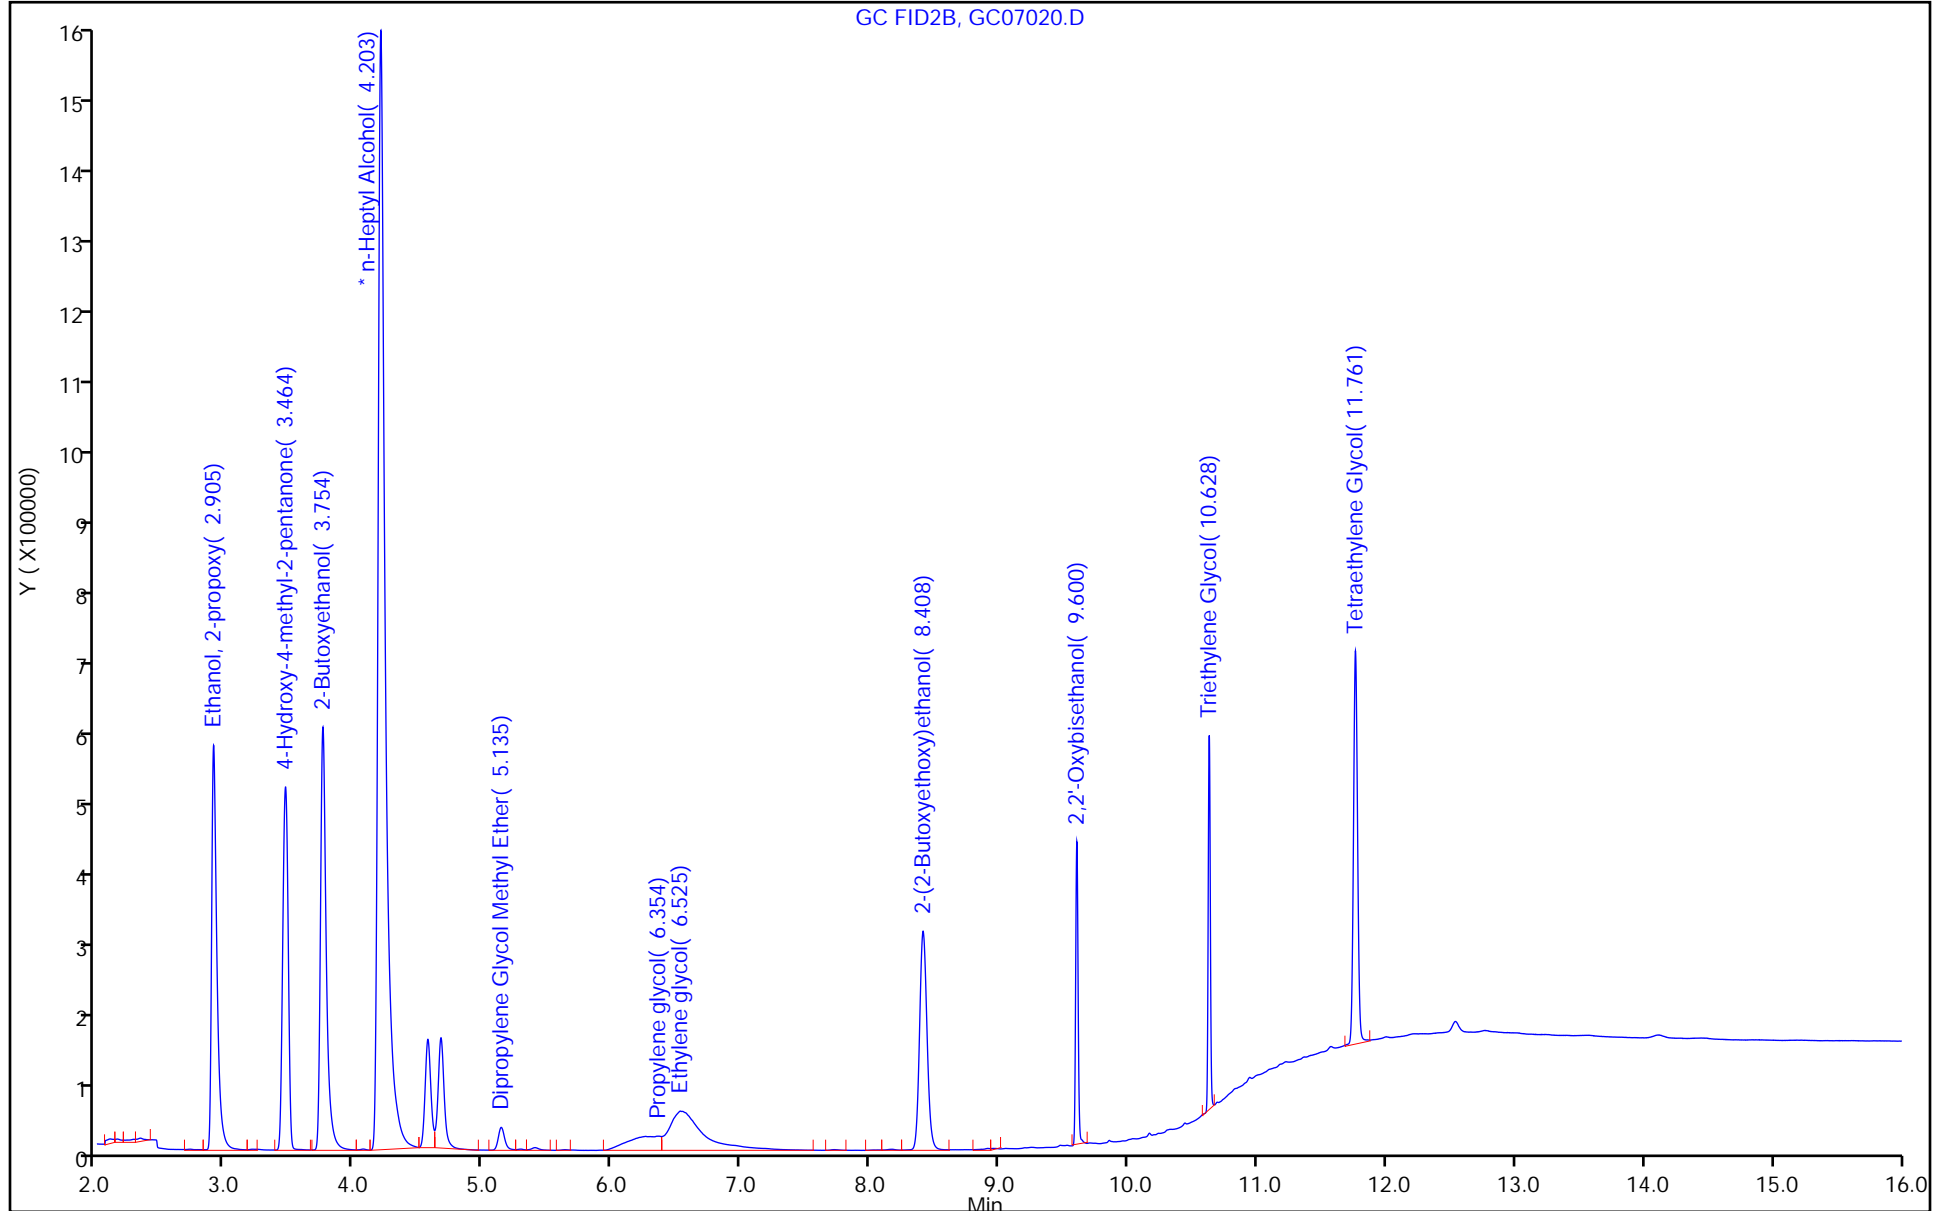

Eurofins Savannah


Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07020.D
Injection Date: 07-Mar-2023 20:20:49 Instrument ID: CVGG2
Lims ID: icv gly
Client ID:
Operator ID: ALS Bottle#: 0 Worklist Smp#: 12
Injection Vol: 1.0 ul Dil. Factor: 1.0000
Method: 8015_GLY_VGG Limit Group: 8015C_DAI
Column: J&W DB WAX (0.45 mm) Detector: GC FID2B

6 Propylene glycol, CAS: 57-55-6

Signal: 1


RT: 6.35
Area: 62366
Amount: 3.363919
Amount Units: ug/ml

Processing Integration Results

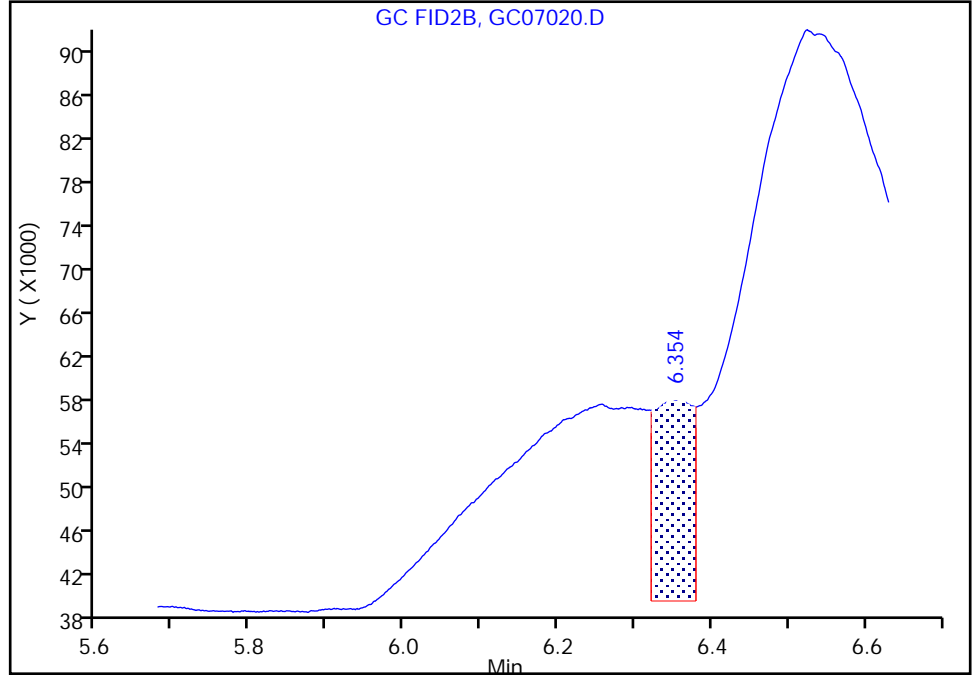

RT: 6.35
Area: 332520
Amount: 18.997137
Amount Units: ug/ml

Manual Integration Results

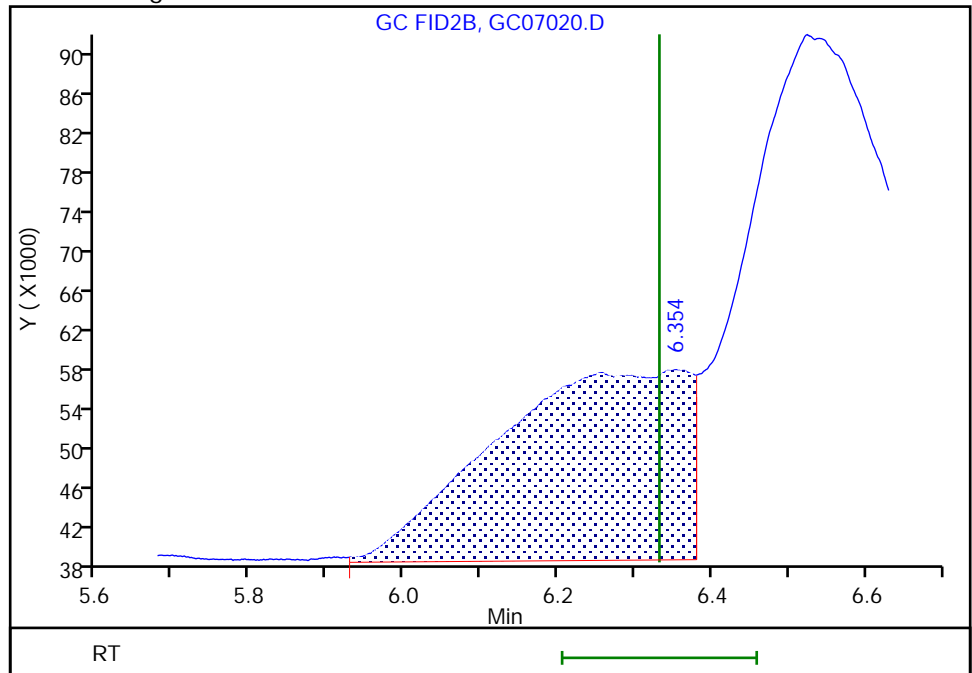

Eurofins Savannah


Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07020.D
Injection Date: 07-Mar-2023 20:20:49 Instrument ID: CVGG2
Lims ID: icv gly
Client ID:
Operator ID: ALS Bottle#: 0 Worklist Smp#: 12
Injection Vol: 1.0 ul Dil. Factor: 1.0000
Method: 8015_GLY_VGG Limit Group: 8015C_DAI
Column: J&W DB WAX (0.45 mm) Detector: GC FID2B

7 Ethylene glycol, CAS: 107-21-1

Signal: 1


RT: 6.52
Area: 865103
Amount: 18.697402
Amount Units: ug/ml

Processing Integration Results

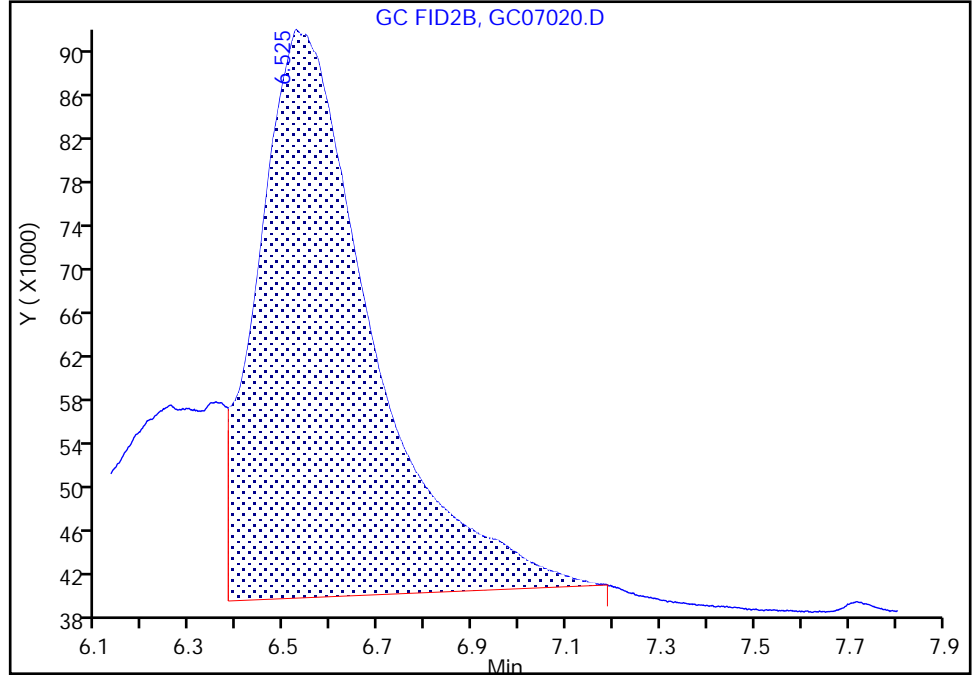

RT: 6.52
Area: 973933
Amount: 21.035088
Amount Units: ug/ml

Manual Integration Results

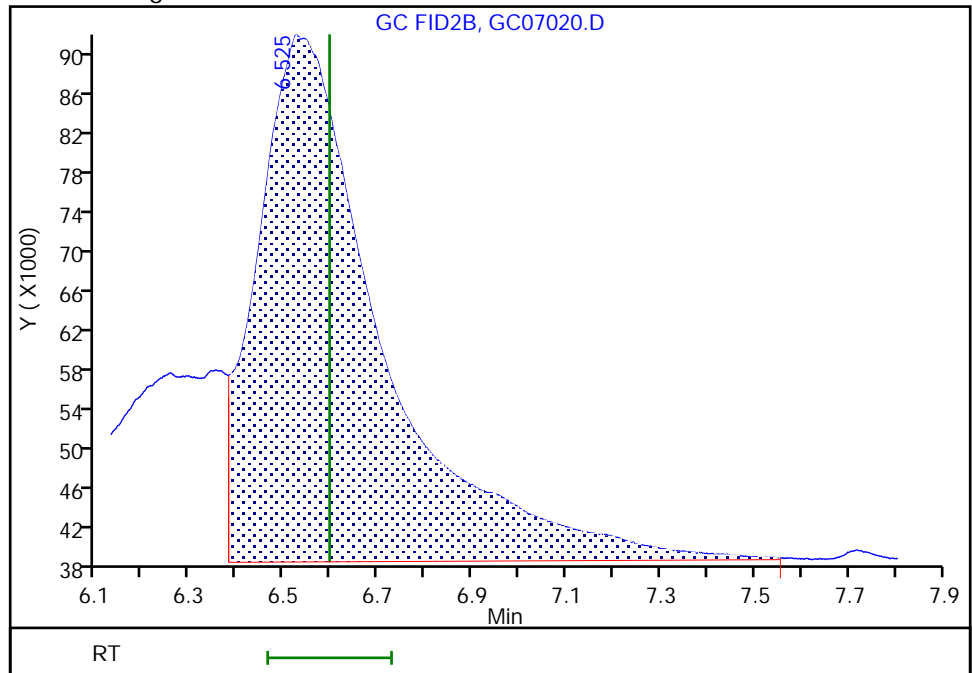

Reviewer: SWK1, 08-Mar-2023 10:50:27
Audit Action: Assigned New Baseline

Audit Reason: Baseline Smoothing

FORM VII
GC SEMI VOA CONTINUING CALIBRATION DATA

Lab Name: Eurofins Savannah Job No.: 580-124266-1
 SDG No.: _____
 Lab Sample ID: CCV 680-766428/32 Calibration Date: 03/08/2023 04:08
 Instrument ID: CVGG2 Calib Start Date: 03/07/2023 17:36
 GC Column: J&W DB WAX ID: 0.45 (mm) Calib End Date: 03/07/2023 19:57
 Lab File ID: GC07040.D Conc. Units: mg/L

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Ethanol, 2-propoxy	Lin1		0.6406		22.7	20.0	13.4	20.0
4-Hydroxy-4-methyl-2-pentano ne	Lin1		0.5933		22.3	20.0	11.5	20.0
2-Butoxyethanol	Lin2		0.7061		21.6	20.0	8.0	20.0
Dipropylene Glycol Methyl Ether	Lin1		0.0489		23.9	20.0	19.6	20.0
Propylene glycol	Lin1		0.1141		15.0	20.0	-24.9*	20.0
Ethylene glycol	Lin1		0.4130		21.0	20.0	5.2	20.0
2-(2-Butoxyethoxy)ethanol	Lin2		0.5350		22.9	20.0	14.5	20.0
2,2'-Oxybisethanol	Lin1		0.1685		13.1	20.0	-34.4*	20.0
Triethylene Glycol	Lin1		0.1286		9.77	20.0	-51.1*	20.0
Tetraethylene Glycol	Lin1		0.0452		5.18	40.0	-87.1*	20.0

FORM VII
GC SEMI VOA CONTINUING CALIBRATION RETENTION TIME SUMMARY

Lab Name: Eurofins Savannah Job No.: 580-124266-1
 SDG No.: _____
 Lab Sample ID: CCV 680-766428/32 Calibration Date: 03/08/2023 04:08
 Instrument ID: CVGG2 Calib Start Date: 03/07/2023 17:36
 GC Column: J&W DB WAX ID: 0.45 (mm) Calib End Date: 03/07/2023 19:57
 Lab File ID: GC07040.D

Analyte	RT	RT WINDOW	
		FROM	TO
Ethanol, 2-propoxy	2.91	2.85	2.97
4-Hydroxy-4-methyl-2-pentanone	3.47	3.40	3.54
2-Butoxyethanol	3.76	3.68	3.83
Dipropylene Glycol Methyl Ether	5.14	5.04	5.24
Propylene glycol	6.35	6.22	6.48
Ethylene glycol	6.58	6.45	6.71
2-(2-Butoxyethoxy)ethanol	8.41	8.24	8.58
2,2'-Oxybisethanol	9.60	9.41	9.80
Triethylene Glycol	10.63	10.42	10.85
Tetraethylene Glycol	11.78	11.55	12.02

Eurofins Savannah
Target Compound Quantitation Report

Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07040.D
 Lims ID: ccv g4
 Client ID:
 Sample Type: CCV
 Inject. Date: 08-Mar-2023 04:08:55 ALS Bottle#: 0 Worklist Smp#: 32
 Injection Vol: 1.0 ul Dil. Factor: 1.0000
 Sample Info: 680-0084239-032
 Operator ID: Instrument ID: CVGG2
 Sublist: chrom-8015_GLY_VGG*sub2
 Method: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\8015_GLY_VGG.m
 Limit Group: 8015C_DAI
 Last Update: 08-Mar-2023 11:27:15 Calib Date: 07-Mar-2023 19:57:23
 Integrator: Falcon
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07019.D
 Column 1 : J&W DB WAX (0.45 mm) Det: GC FID2B
 Process Host: CTX1619

First Level Reviewer: SWK1 Date: 08-Mar-2023 11:20:06

RT (min.)	Exp RT (min.)	Dlt RT (min.)	Response	Cal Amt ug/ml	OnCol Amt ug/ml	Flags
1 Ethanol, 2-propoxy						
2.912	2.912	0.000	1570009	20.0	22.7	
2 4-Hydroxy-4-methyl-2-pentanone						
3.469	3.469	0.000	1454107	20.0	22.3	
3 2-Butoxyethanol						
3.755	3.755	0.000	1730383	20.0	21.6	
* 4 n-Heptyl Alcohol						
4.200	4.200	0.000	6126690	50.0	50.0	
5 Dipropylene Glycol Methyl Ether						
5.138	5.138	0.000	119921	20.0	23.9	
6 Propylene glycol						
6.349	6.349	0.000	279572	20.0	15.0	
7 Ethylene glycol						
6.577	6.577	0.000	1012169	20.0	21.0	
8 2-(2-Butoxyethoxy)ethanol						
8.407	8.407	0.000	1311158	20.0	22.9	
9 2,2'-Oxybisethanol						
9.604	9.604	0.000	412879	20.0	13.1	
10 Triethylene Glycol						
10.634	10.634	0.000	315045	20.0	9.77	
11 Tetraethylene Glycol						
11.782	11.782	0.000	221782	40.0	5.18	

QC Flag Legend
Processing Flags

Reagents:

SG_Gly_CAL_00048

Amount Added: 10.00

Units: uL

SG_GLY_ISTD_00106

Amount Added: 10.00

Units: uL

Run Reagent

Eurofins Savannah

Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07040.D

Injection Date: 08-Mar-2023 04:08:55

Instrument ID: CVGG2

Operator ID:

Lims ID: ccv g4

Worklist Smp#: 32

Client ID:

Injection Vol: 1.0 ul


Dil. Factor: 1.0000

ALS Bottle#: 0

Method: 8015_GLY_VGG

Limit Group: 8015C_DAI

Column: J&W DB WAX (0.45 mm)

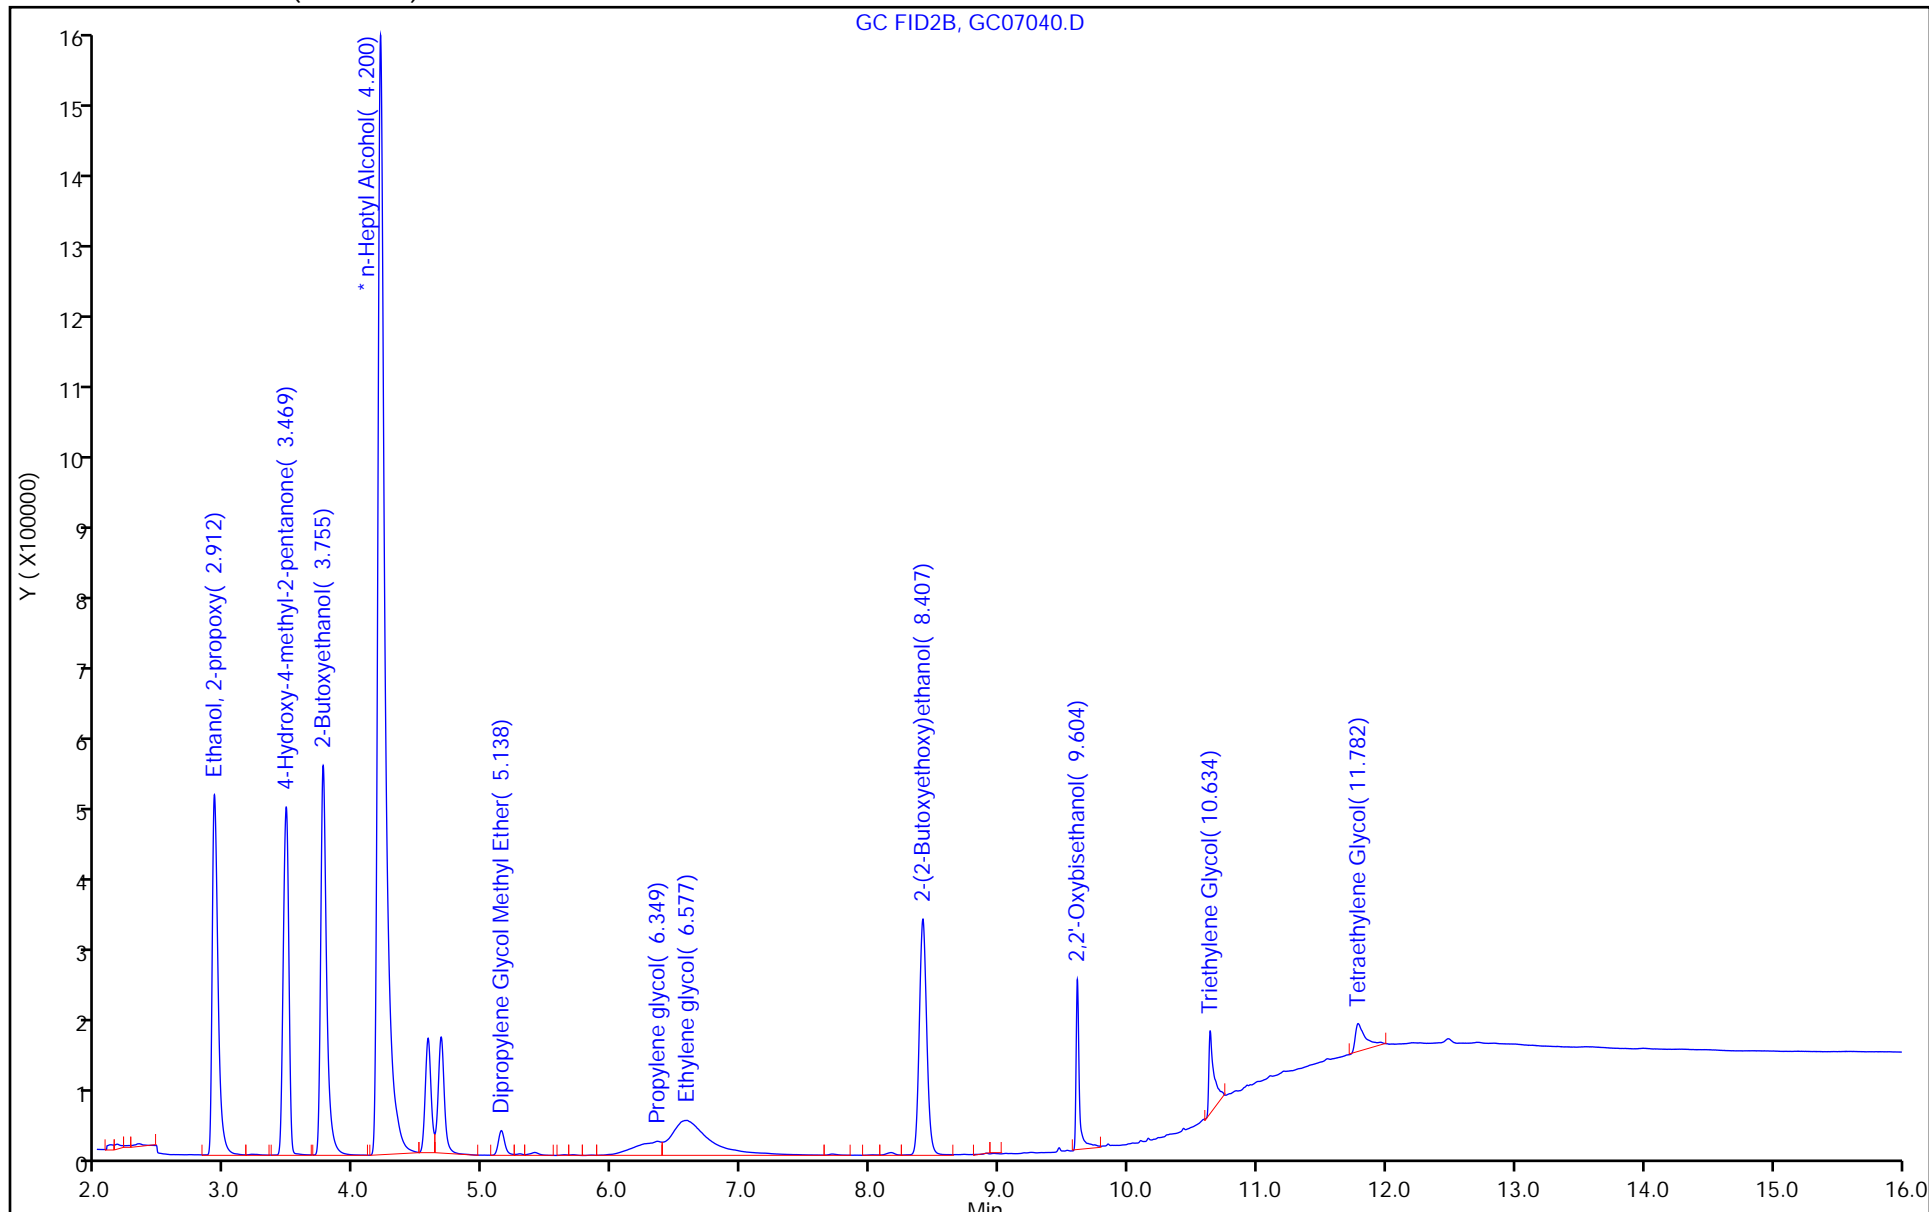

FORM VII
GC SEMI VOA CONTINUING CALIBRATION DATA

Lab Name: Eurofins Savannah Job No.: 580-124266-1
 SDG No.: _____
 Lab Sample ID: CCV 680-766428/40 Calibration Date: 03/08/2023 07:15
 Instrument ID: CVGG2 Calib Start Date: 03/07/2023 17:36
 GC Column: J&W DB WAX ID: 0.45 (mm) Calib End Date: 03/07/2023 19:57
 Lab File ID: GC07048.D Conc. Units: mg/L

ANALYTE	CURVE TYPE	AVE RRF	RRF	MIN RRF	CALC AMOUNT	SPIKE AMOUNT	%D	MAX %D
Ethanol, 2-propoxy	Lin1		0.5867		20.5	20.0	2.6	20.0
4-Hydroxy-4-methyl-2-pentano ne	Lin1		0.5402		20.0	20.0	0.2	20.0
2-Butoxyethanol	Lin2		0.6573		20.0	20.0	-0.2	20.0
Dipropylene Glycol Methyl Ether	Lin1		0.0426		20.5	20.0	2.5	20.0
Propylene glycol	Lin1		0.0915		11.7	20.0	-41.6*	20.0
Ethylene glycol	Lin1		0.4591		23.5	20.0	17.4	20.0
2-(2-Butoxyethoxy)ethanol	Lin2		0.5087		21.7	20.0	8.3	20.0
2,2'-Oxybisethanol	Lin1		0.2051		16.3	20.0	-18.6	20.0
Triethylene Glycol	Lin1		0.1360		10.4	20.0	-47.8*	20.0
Tetraethylene Glycol	Lin1		0.0560		7.05	40.0	-82.4*	20.0

FORM VII
GC SEMI VOA CONTINUING CALIBRATION RETENTION TIME SUMMARY

Lab Name: Eurofins Savannah Job No.: 580-124266-1
 SDG No.: _____
 Lab Sample ID: CCV 680-766428/40 Calibration Date: 03/08/2023 07:15
 Instrument ID: CVGG2 Calib Start Date: 03/07/2023 17:36
 GC Column: J&W DB WAX ID: 0.45 (mm) Calib End Date: 03/07/2023 19:57
 Lab File ID: GC07048.D

Analyte	RT	RT WINDOW	
		FROM	TO
Ethanol, 2-propoxy	2.91	2.86	2.97
4-Hydroxy-4-methyl-2-pentanone	3.47	3.40	3.54
2-Butoxyethanol	3.76	3.68	3.83
Dipropylene Glycol Methyl Ether	5.14	5.03	5.24
Propylene glycol	6.33	6.21	6.46
Ethylene glycol	6.60	6.46	6.73
2-(2-Butoxyethoxy)ethanol	8.41	8.24	8.58
2,2'-Oxybisethanol	9.60	9.41	9.80
Triethylene Glycol	10.64	10.42	10.85
Tetraethylene Glycol	11.79	11.55	12.02

Eurofins Savannah
Target Compound Quantitation Report

Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07048.D
 Lims ID: ccv g4
 Client ID:
 Sample Type: CCV
 Inject. Date: 08-Mar-2023 07:15:18 ALS Bottle#: 0 Worklist Smp#: 40
 Injection Vol: 1.0 ul Dil. Factor: 1.0000
 Sample Info: 680-0084239-040
 Operator ID: Instrument ID: CVGG2
 Sublist: chrom-8015_GLY_VGG*sub2
 Method: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\8015_GLY_VGG.m
 Limit Group: 8015C_DAI
 Last Update: 08-Mar-2023 11:27:16 Calib Date: 07-Mar-2023 19:57:23
 Integrator: Falcon
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07019.D
 Column 1 : J&W DB WAX (0.45 mm) Det: GC FID2B
 Process Host: CTX1619

First Level Reviewer: SWK1 Date: 08-Mar-2023 11:26:45

RT (min.)	Exp RT (min.)	Dlt RT (min.)	Response	Cal Amt ug/ml	OnCol Amt ug/ml	Flags
1 Ethanol, 2-propoxy						
2.914	2.914	0.000	1518110	20.0	20.5	
2 4-Hydroxy-4-methyl-2-pentanone						
3.469	3.469	0.000	1397858	20.0	20.0	
3 2-Butoxyethanol						
3.758	3.758	0.000	1700852	20.0	20.0	
* 4 n-Heptyl Alcohol						
4.204	4.204	0.000	6469378	50.0	50.0	
5 Dipropylene Glycol Methyl Ether						
5.136	5.136	0.000	110177	20.0	20.5	
6 Propylene glycol						
6.332	6.332	0.000	236667	20.0	11.7	
7 Ethylene glycol						
6.595	6.595	0.000	1188062	20.0	23.5	
8 2-(2-Butoxyethoxy)ethanol						
8.407	8.407	0.000	1316483	20.0	21.7	
9 2,2'-Oxybisethanol						
9.604	9.604	0.000	530689	20.0	16.3	
10 Triethylene Glycol						
10.637	10.637	0.000	351847	20.0	10.4	
11 Tetraethylene Glycol						
11.789	11.789	0.000	289590	40.0	7.05	

QC Flag Legend
Processing Flags

Reagents:

SG_Gly_CAL_00048

Amount Added: 10.00

Units: uL

SG_GLY_ISTD_00106

Amount Added: 10.00

Units: uL

Run Reagent

Eurofins Savannah

Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07048.D

Injection Date: 08-Mar-2023 07:15:18

Instrument ID: CVGG2

Operator ID:

Lims ID: ccv g4

Worklist Smp#: 40

Client ID:

Injection Vol: 1.0 ul


Dil. Factor: 1.0000

ALS Bottle#: 0

Method: 8015_GLY_VGG

Limit Group: 8015C_DAI

Column: J&W DB WAX (0.45 mm)

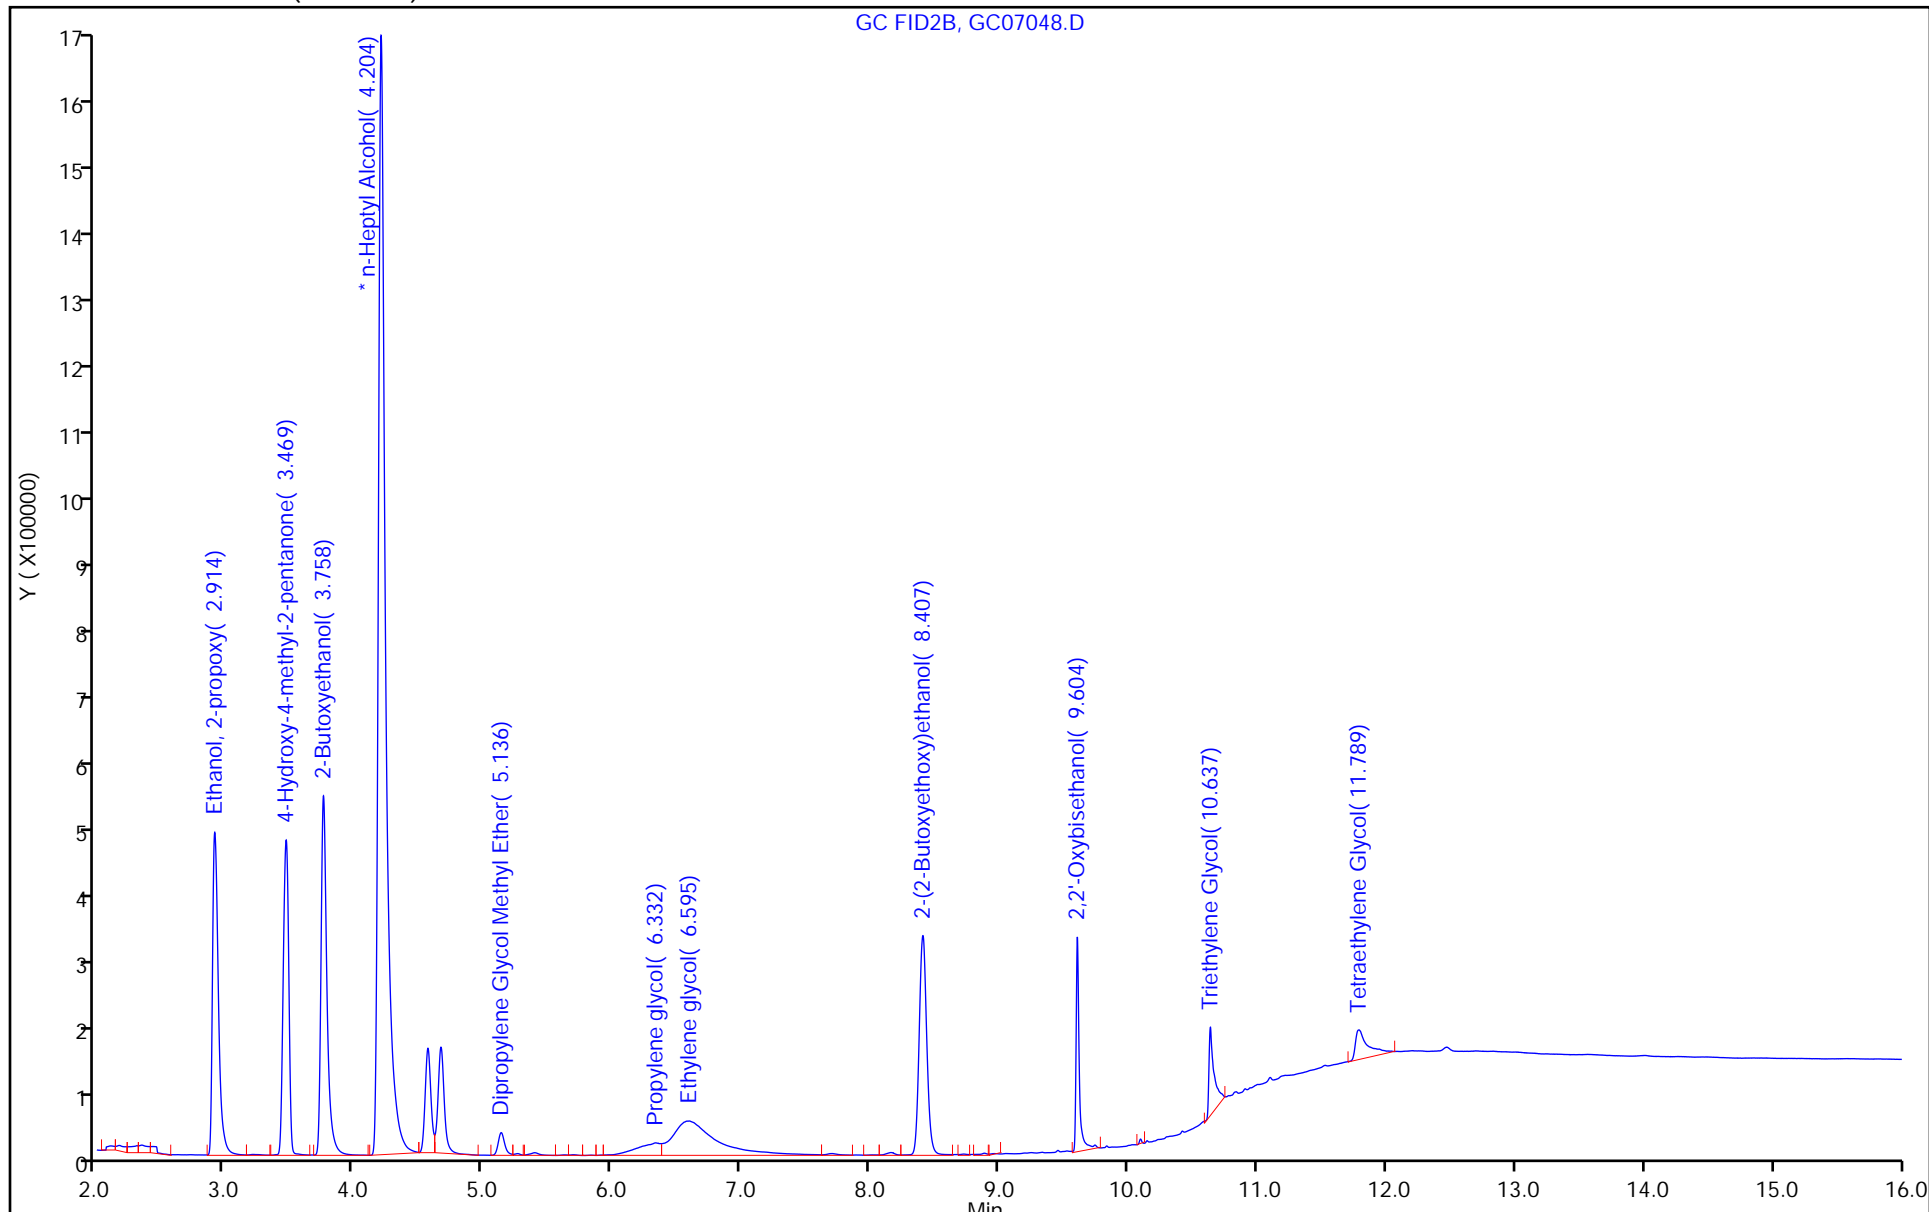

FORM I
GC SEMI VOA ORGANICS ANALYSIS DATA SHEET

Lab Name: Eurofins Savannah Job No.: 580-124266-1
 SDG No.: _____
 Client Sample ID: _____ Lab Sample ID: MB 680-766428/17
 Matrix: Water Lab File ID: GC07025.D
 Analysis Method: 8015C GLY Date Collected: _____
 Extraction Method: _____ Date Extracted: _____
 Sample wt/vol: 1(mL) Date Analyzed: 03/07/2023 22:18
 Con. Extract Vol.: 1(mL) Dilution Factor: 1
 Injection Volume: 1(uL) GC Column: J&W DB WAX ID: 0.45(mm)
 % Moisture: _____ % Solids: _____ GPC Cleanup: (Y/N) N
 Cleanup Factor: _____
 Analysis Batch No.: 766428 Units: mg/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
112-34-5	2-(2-Butoxyethoxy)ethanol	3.0	U M	5.0	3.0	1.1

Eurofins Savannah
Target Compound Quantitation Report

Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07025.D
 Lims ID: mb
 Client ID:
 Sample Type: MB
 Inject. Date: 07-Mar-2023 22:18:03 ALS Bottle#: 0 Worklist Smp#: 17
 Injection Vol: 1.0 ul Dil. Factor: 1.0000
 Sample Info: 680-0084239-017
 Operator ID: Instrument ID: CVGG2
 Method: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\8015_GLY_VGG.m
 Limit Group: 8015C_DAI
 Last Update: 08-Mar-2023 11:26:45 Calib Date: 07-Mar-2023 19:57:23
 Integrator: Falcon
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07019.D
 Column 1 : J&W DB WAX (0.45 mm) Det: GC FID2B
 Process Host: CTX1619

First Level Reviewer: SWK1 Date: 08-Mar-2023 11:13:51

RT (min.)	Exp RT (min.)	Dlt RT (min.)	Response	Cal Amt ug/ml	OnCol Amt ug/ml	Flags
-----------	---------------	---------------	----------	---------------	-----------------	-------

* 4 n-Heptyl Alcohol
 4.204 4.204 0.000 6806623 50.0 50.0
 10 Triethylene Glycol 7
 10.628 10.637 -0.009 84069 1.02 7
 LOD = 1.40

QC Flag Legend

Processing Flags

7 - Failed Limit of Detection

Reagents:

SG_GLY_ISTD_00106 Amount Added: 10.00 Units: uL Run Reagent

Eurofins Savannah

Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07025.D

Injection Date: 07-Mar-2023 22:18:03

Instrument ID: CVGG2

Operator ID:

Lims ID: mb

Worklist Smp#: 17

Client ID:

Injection Vol: 1.0 ul


Dil. Factor: 1.0000

ALS Bottle#: 0

Method: 8015_GLY_VGG

Limit Group: 8015C_DAI

Column: J&W DB WAX (0.45 mm)

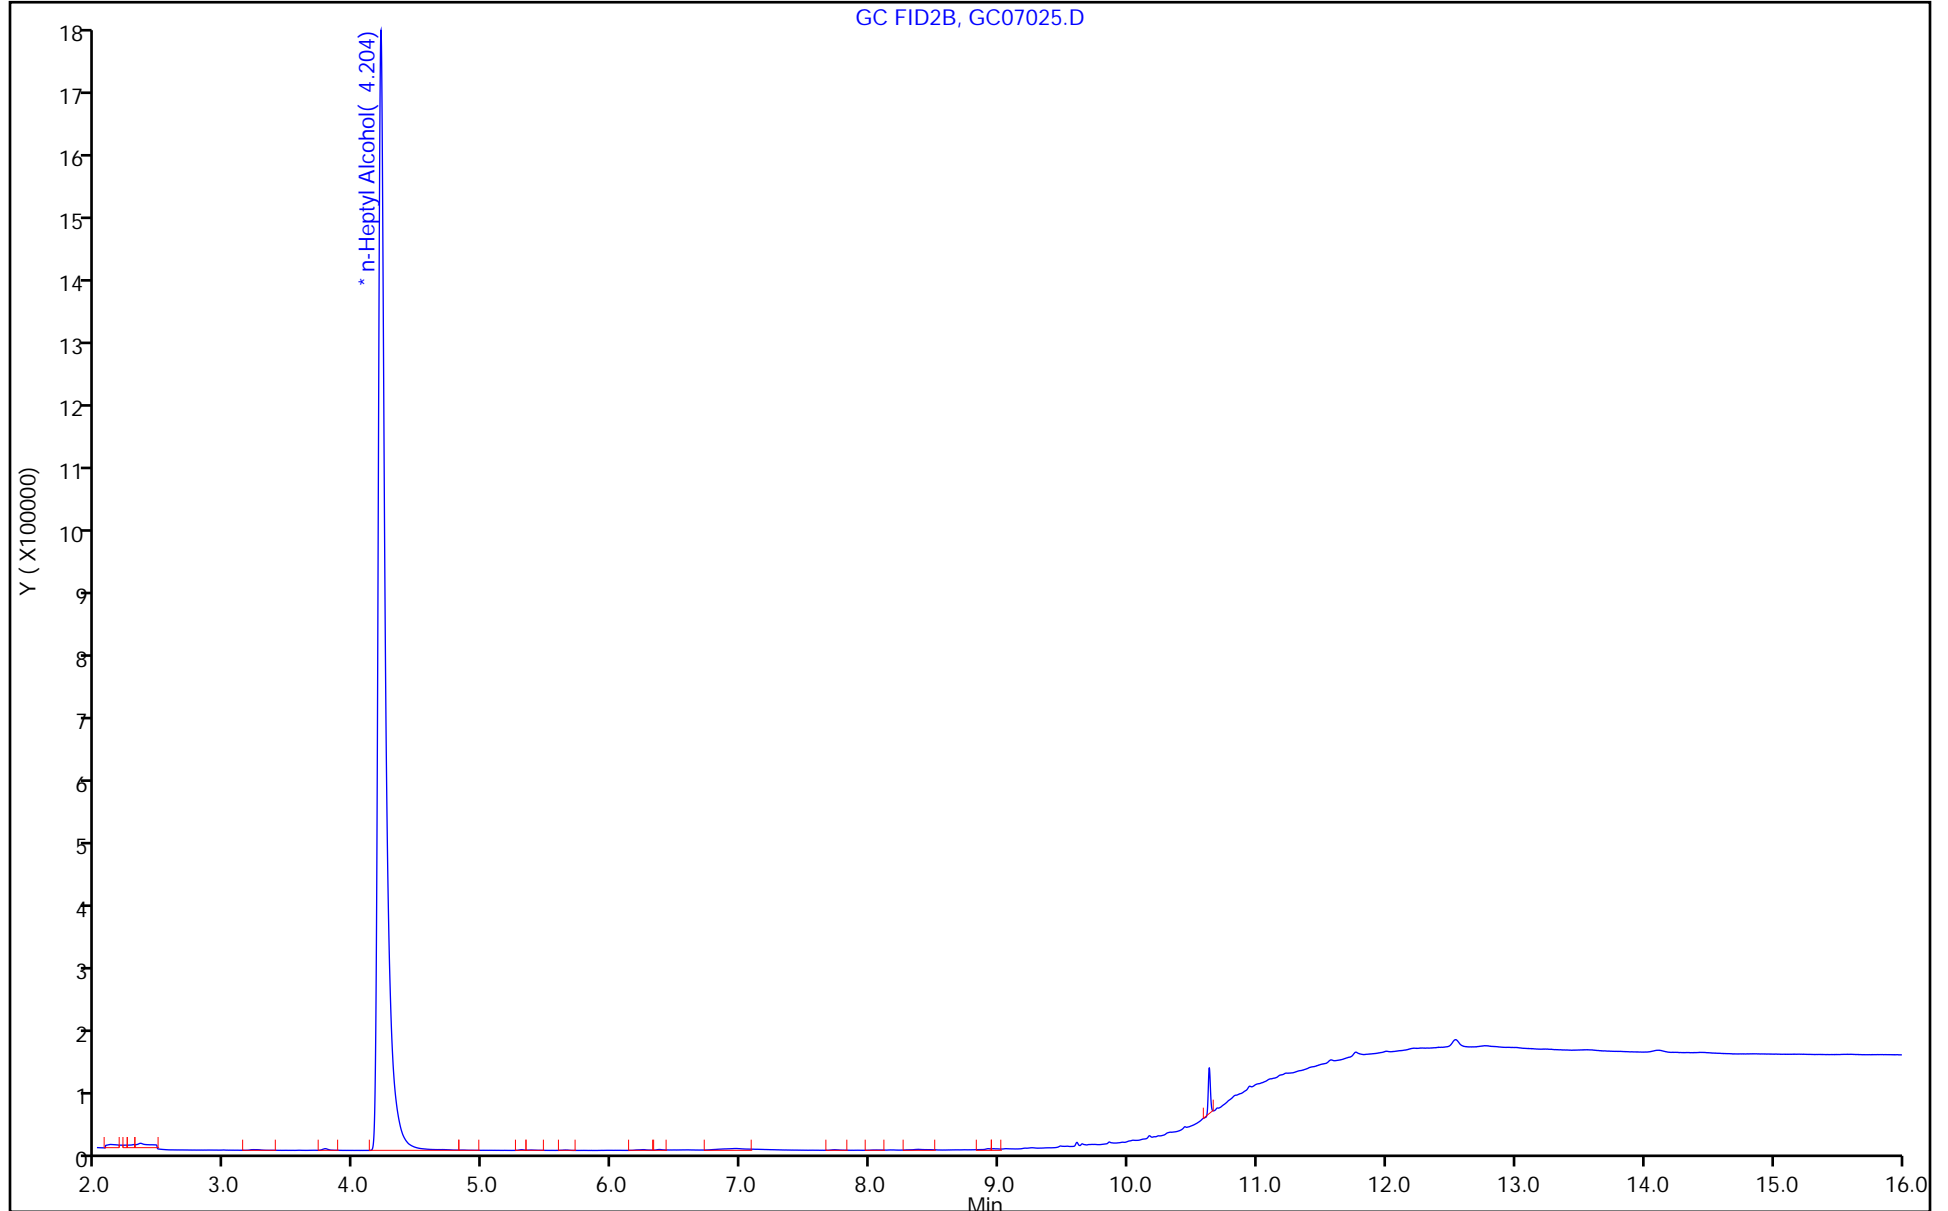

FORM I
GC SEMI VOA ORGANICS ANALYSIS DATA SHEET

Lab Name: Eurofins Savannah Job No.: 580-124266-1
 SDG No.: _____
 Client Sample ID: _____ Lab Sample ID: LCS 680-766428/13
 Matrix: Water Lab File ID: GC07021.D
 Analysis Method: 8015C GLY Date Collected: _____
 Extraction Method: _____ Date Extracted: _____
 Sample wt/vol: 1(mL) Date Analyzed: 03/07/2023 20:44
 Con. Extract Vol.: 1(mL) Dilution Factor: 1
 Injection Volume: 1(uL) GC Column: J&W DB WAX ID: 0.45(mm)
 % Moisture: _____ % Solids: _____ GPC Cleanup: (Y/N) N
 Cleanup Factor: _____
 Analysis Batch No.: 766428 Units: mg/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
112-34-5	2-(2-Butoxyethoxy)ethanol	21.5		5.0	3.0	1.1

Eurofins Savannah
Target Compound Quantitation Report

Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07021.D
 Lims ID: lcs
 Client ID:
 Sample Type: LCS
 Inject. Date: 07-Mar-2023 20:44:15 ALS Bottle#: 0 Worklist Smp#: 13
 Injection Vol: 1.0 ul Dil. Factor: 1.0000
 Sample Info: 680-0084239-013
 Operator ID: Instrument ID: CVGG2
 Method: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\8015_GLY_VGG.m
 Limit Group: 8015C_DAI
 Last Update: 08-Mar-2023 11:27:12 Calib Date: 07-Mar-2023 19:57:23
 Integrator: Falcon
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07019.D
 Column 1 : J&W DB WAX (0.45 mm) Det: GC FID2B
 Process Host: CTX1619

First Level Reviewer: SWK1 Date: 08-Mar-2023 11:13:29

RT (min.)	Exp RT (min.)	Diff RT (min.)	Response	Cal Amt ug/ml	OnCol Amt ug/ml	Flags
1 Ethanol, 2-propoxy						
2.906	2.914	-0.008	1470548	20.0	22.6	
2 4-Hydroxy-4-methyl-2-pentanone						
3.465	3.469	-0.004	1379918	20.0	22.6	
3 2-Butoxyethanol						
3.754	3.758	-0.004	1693138	20.0	22.6	
* 4 n-Heptyl Alcohol						
4.203	4.204	-0.001	5749580	50.0	50.0	
5 Dipropylene Glycol Methyl Ether						
5.137	5.136	0.001	104983	20.0	22.2	
6 Propylene glycol						
6.355	6.332	0.023	335233	20.0	19.7	M
7 Ethylene glycol						
6.534	6.595	-0.061	991125	20.0	22.0	
8 2-(2-Butoxyethoxy)ethanol						
8.409	8.407	0.002	1160731	20.0	21.5	
9 2,2'-Oxybisethanol						
9.600	9.604	-0.004	579897	20.0	20.4	
10 Triethylene Glycol						
10.627	10.637	-0.010	618946	20.0	22.4	
11 Tetraethylene Glycol						
11.762	11.789	-0.027	1267045	40.0	45.5	

QC Flag Legend

Processing Flags

Review Flags

M - Manually Integrated

Reagents:

SG_GlyICV_00055

Amount Added: 10.00

Units: uL

SG_GLY_ISTD_00106

Amount Added: 10.00

Units: uL

Run Reagent

Eurofins Savannah

Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07021.D

Injection Date: 07-Mar-2023 20:44:15

Instrument ID: CVGG2

Operator ID:

Lims ID: lcs

Worklist Smp#: 13

Client ID:

Injection Vol: 1.0 ul


Dil. Factor: 1.0000

ALS Bottle#: 0

Method: 8015_GLY_VGG

Limit Group: 8015C_DAI

Column: J&W DB WAX (0.45 mm)

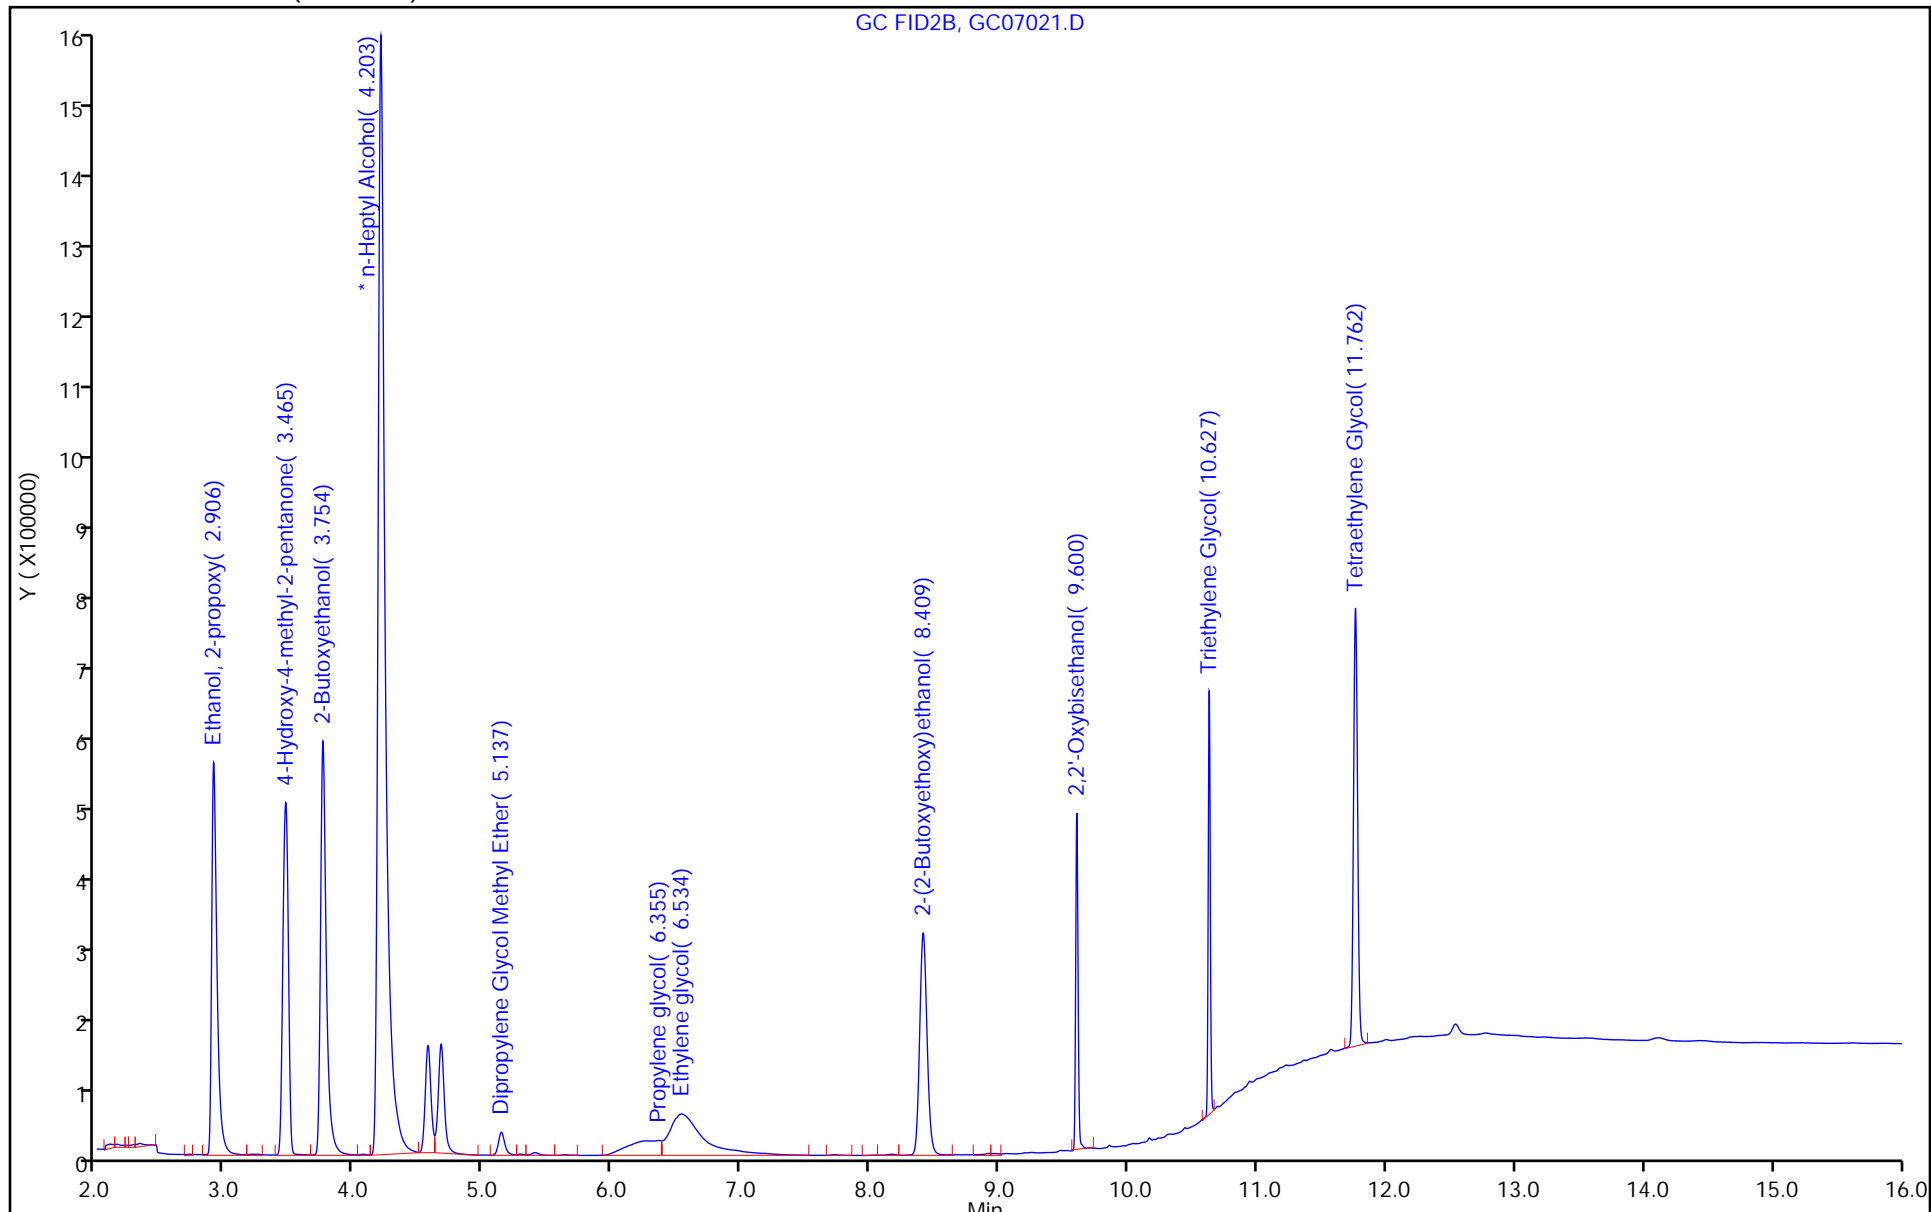

FORM I
GC SEMI VOA ORGANICS ANALYSIS DATA SHEET

Lab Name: Eurofins Savannah Job No.: 580-124266-1
 SDG No.: _____
 Client Sample ID: _____ Lab Sample ID: LCSD 680-766428/14
 Matrix: Water Lab File ID: GC07022.D
 Analysis Method: 8015C GLY Date Collected: _____
 Extraction Method: _____ Date Extracted: _____
 Sample wt/vol: 1(mL) Date Analyzed: 03/07/2023 21:07
 Con. Extract Vol.: 1(mL) Dilution Factor: 1
 Injection Volume: 1(uL) GC Column: J&W DB WAX ID: 0.45(mm)
 % Moisture: _____ % Solids: _____ GPC Cleanup: (Y/N) N
 Cleanup Factor: _____
 Analysis Batch No.: 766428 Units: mg/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
112-34-5	2-(2-Butoxyethoxy)ethanol	23.1		5.0	3.0	1.1

Eurofins Savannah
Target Compound Quantitation Report

Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07022.D
 Lims ID: lcsd
 Client ID:
 Sample Type: LCSD
 Inject. Date: 07-Mar-2023 21:07:46 ALS Bottle#: 0 Worklist Smp#: 14
 Injection Vol: 1.0 ul Dil. Factor: 1.0000
 Sample Info: 680-0084239-014
 Operator ID: Instrument ID: CVGG2
 Method: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\8015_GLY_VGG.m
 Limit Group: 8015C_DAI
 Last Update: 08-Mar-2023 11:27:12 Calib Date: 07-Mar-2023 19:57:23
 Integrator: Falcon
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07019.D
 Column 1 : J&W DB WAX (0.45 mm) Det: GC FID2B
 Process Host: CTX1619

First Level Reviewer: SWK1 Date: 08-Mar-2023 11:13:41

RT (min.)	Exp RT (min.)	Diff RT (min.)	Response	Cal Amt ug/ml	OnCol Amt ug/ml	Flags
1 Ethanol, 2-propoxy						
2.908	2.914	-0.006	1631152	20.0	24.9	
2 4-Hydroxy-4-methyl-2-pentanone						
3.469	3.469	0.000	1573763	20.0	25.6	
3 2-Butoxyethanol						
3.754	3.758	-0.004	1851844	20.0	24.4	
* 4 n-Heptyl Alcohol						
4.200	4.204	-0.004	5861610	50.0	50.0	
5 Dipropylene Glycol Methyl Ether						
5.140	5.136	0.004	111113	20.0	23.1	
6 Propylene glycol						
6.353	6.332	0.021	296468	20.0	16.8	M
7 Ethylene glycol						
6.539	6.595	-0.056	844057	20.0	18.2	
8 2-(2-Butoxyethoxy)ethanol						
8.409	8.407	0.002	1264524	20.0	23.1	
9 2,2'-Oxybisethanol						
9.601	9.604	-0.003	448103	20.0	15.1	
10 Triethylene Glycol						
10.628	10.637	-0.009	471568	20.0	16.3	
11 Tetraethylene Glycol						
11.762	11.789	-0.027	946494	40.0	32.6	

QC Flag Legend

Processing Flags

Review Flags

M - Manually Integrated

Reagents:

SG_GlyICV_00055

Amount Added: 10.00

Units: uL

SG_GLY_ISTD_00106

Amount Added: 10.00

Units: uL

Run Reagent

Eurofins Savannah

Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07022.D

Injection Date: 07-Mar-2023 21:07:46

Instrument ID: CVGG2

Operator ID:

Lims ID: lcsd

Worklist Smp#: 14

Client ID:

Injection Vol: 1.0 ul


Dil. Factor: 1.0000

ALS Bottle#: 0

Method: 8015_GLY_VGG

Limit Group: 8015C_DAI

Column: J&W DB WAX (0.45 mm)

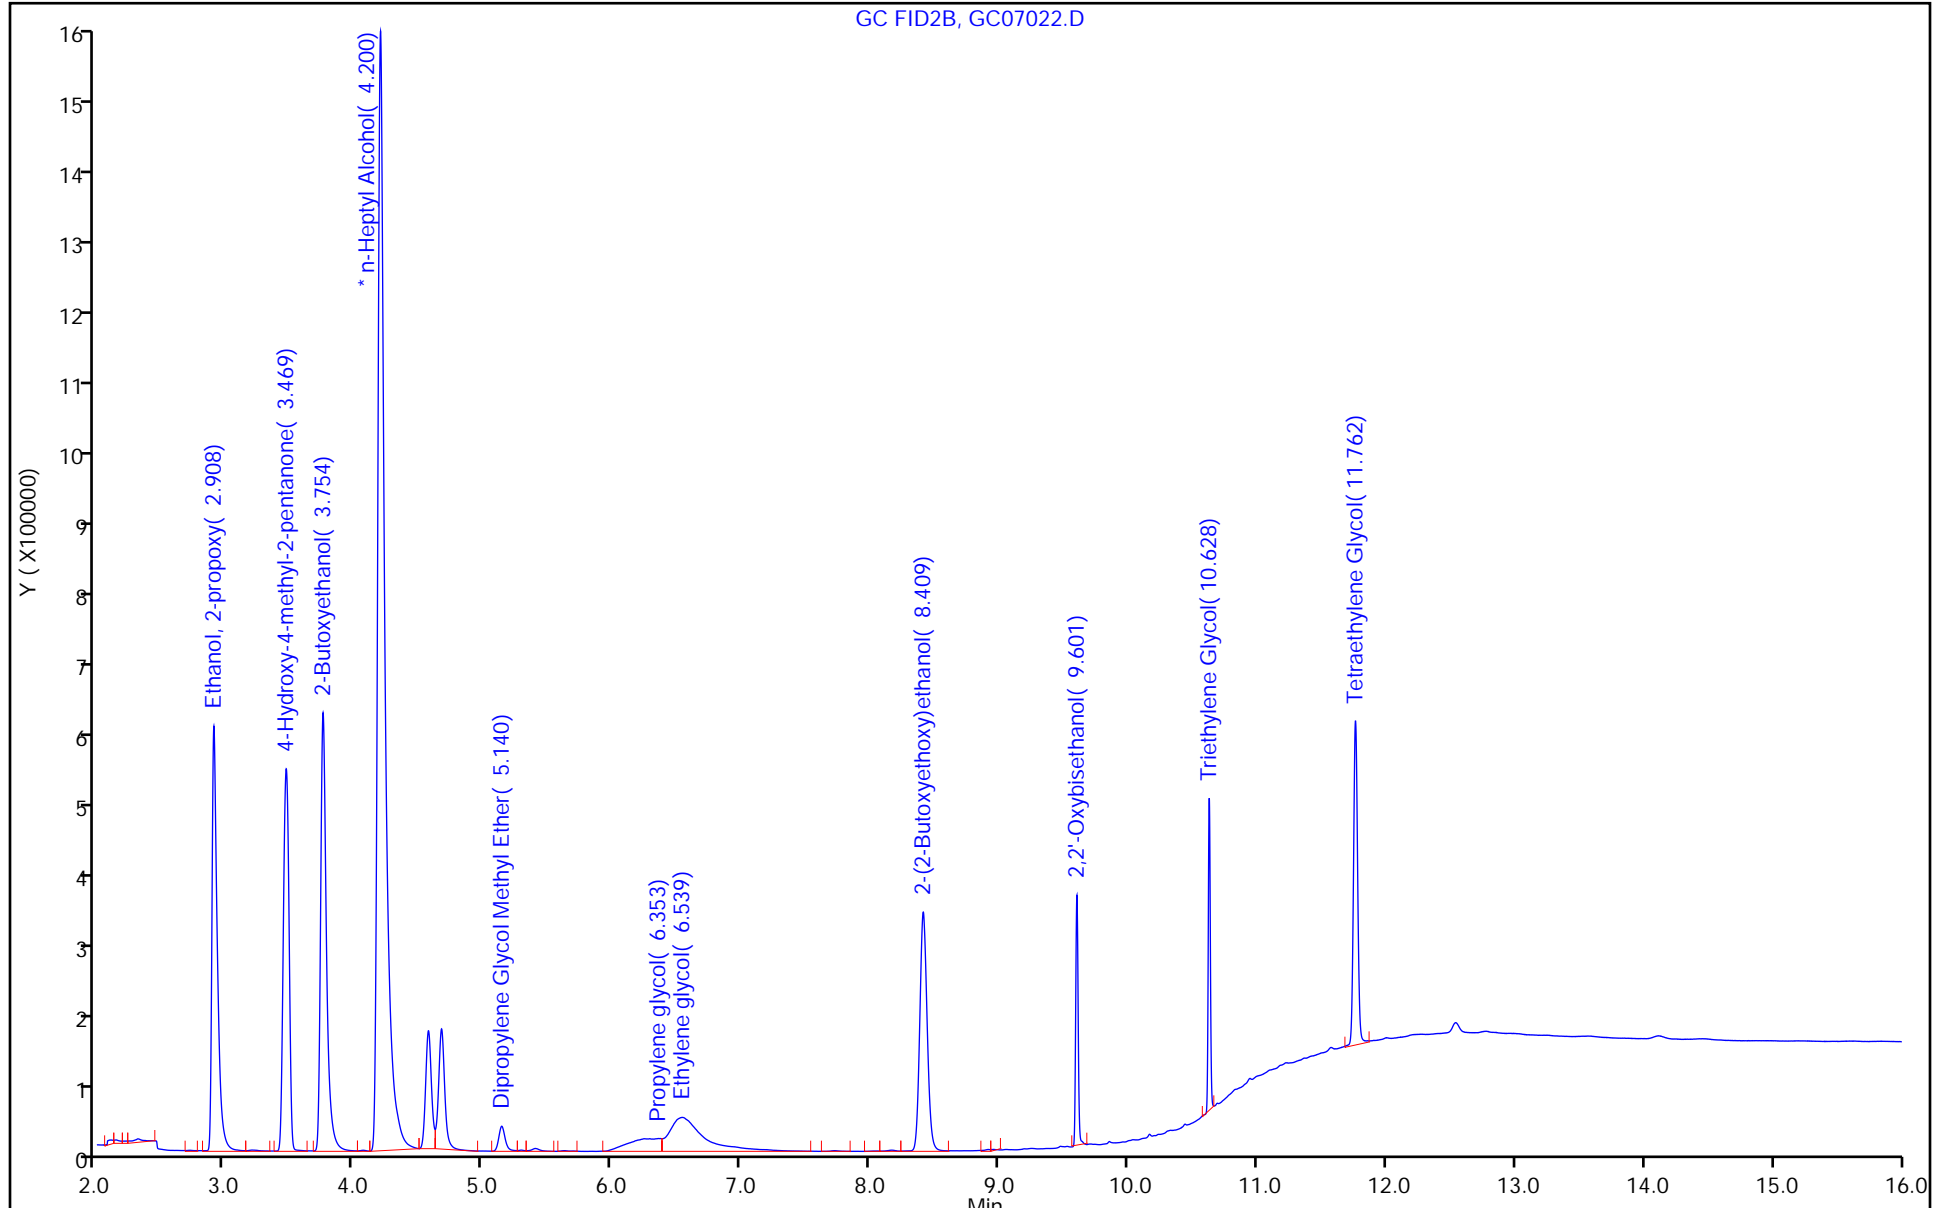

FORM I
GC SEMI VOA ORGANICS ANALYSIS DATA SHEET

Lab Name: Eurofins Savannah Job No.: 580-124266-1
SDG No.: _____
Client Sample ID: AF-RHWW02-WGN01LF-2302W4 Lab Sample ID: 580-124266-2 MS
MS
Matrix: Water Lab File ID: GC07045.D
Analysis Method: 8015C GLY Date Collected: 03/02/2023 11:10
Extraction Method: _____ Date Extracted: _____
Sample wt/vol: 1(mL) Date Analyzed: 03/08/2023 06:05
Con. Extract Vol.: 1(mL) Dilution Factor: 1
Injection Volume: 1(uL) GC Column: J&W DB WAX ID: 0.45(mm)
% Moisture: _____ % Solids: _____ GPC Cleanup: (Y/N) N
Cleanup Factor: _____
Analysis Batch No.: 766428 Units: mg/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
112-34-5	2-(2-Butoxyethoxy)ethanol	26.0		5.0	3.0	1.1

Eurofins Savannah
Target Compound Quantitation Report

Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07045.D
 Lims ID: 580-124266-A-2 MS
 Client ID:
 Sample Type: MS
 Inject. Date: 08-Mar-2023 06:05:27 ALS Bottle#: 0 Worklist Smp#: 37
 Injection Vol: 1.0 ul Dil. Factor: 1.0000
 Sample Info: 680-0084239-037
 Operator ID: Instrument ID: CVGG2
 Method: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\8015_GLY_VGG.m
 Limit Group: 8015C_DAI
 Last Update: 08-Mar-2023 11:26:45 Calib Date: 07-Mar-2023 19:57:23
 Integrator: Falcon
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07019.D
 Column 1 : J&W DB WAX (0.45 mm) Det: GC FID2B
 Process Host: CTX1619

First Level Reviewer: SWK1 Date: 08-Mar-2023 11:21:38

RT (min.)	Exp RT (min.)	Dlt RT (min.)	Response	Cal Amt ug/ml	OnCol Amt ug/ml	Flags
-----------	---------------	---------------	----------	---------------	-----------------	-------

1 Ethanol, 2-propoxy						
2.915	2.914	0.001	1683904	20.0	24.1	
2 4-Hydroxy-4-methyl-2-pentanone						
3.475	3.469	0.006	1672421	20.0	25.6	
3 2-Butoxyethanol						
3.758	3.758	0.000	1908900	20.0	23.7	
* 4 n-Heptyl Alcohol						
4.195	4.204	-0.009	6223277	50.0	50.0	
5 Dipropylene Glycol Methyl Ether						
5.144	5.136	0.008	147456	20.0	29.5	
6 Propylene glycol						
6.296	6.332	-0.036	264810	20.0	13.9	M
7 Ethylene glycol						
6.581	6.595	-0.014	876014	20.0	17.8	M
8 2-(2-Butoxyethoxy)ethanol						
8.406	8.407	-0.001	1491485	20.0	26.0	
9 2,2'-Oxybisethanol						
9.604	9.604	0.000	206366	20.0	5.74	
10 Triethylene Glycol						
10.634	10.637	-0.003	42400	20.0	-0.2155	7
LOD = 1.40						

QC Flag Legend

Processing Flags

7 - Failed Limit of Detection

Review Flags

M - Manually Integrated

Reagents:

SG_GlyICV_00055

Amount Added: 10.00

Units: uL

SG_GLY_ISTD_00106

Amount Added: 10.00

Units: uL

Run Reagent

Eurofins Savannah

Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07045.D

Injection Date: 08-Mar-2023 06:05:27

Instrument ID: CVGG2

Operator ID:

Lims ID: 580-124266-A-2 MS

Worklist Smp#: 37

Client ID:

Injection Vol: 1.0 ul


Dil. Factor: 1.0000

ALS Bottle#: 0

Method: 8015_GLY_VGG

Limit Group: 8015C_DAI

Column: J&W DB WAX (0.45 mm)

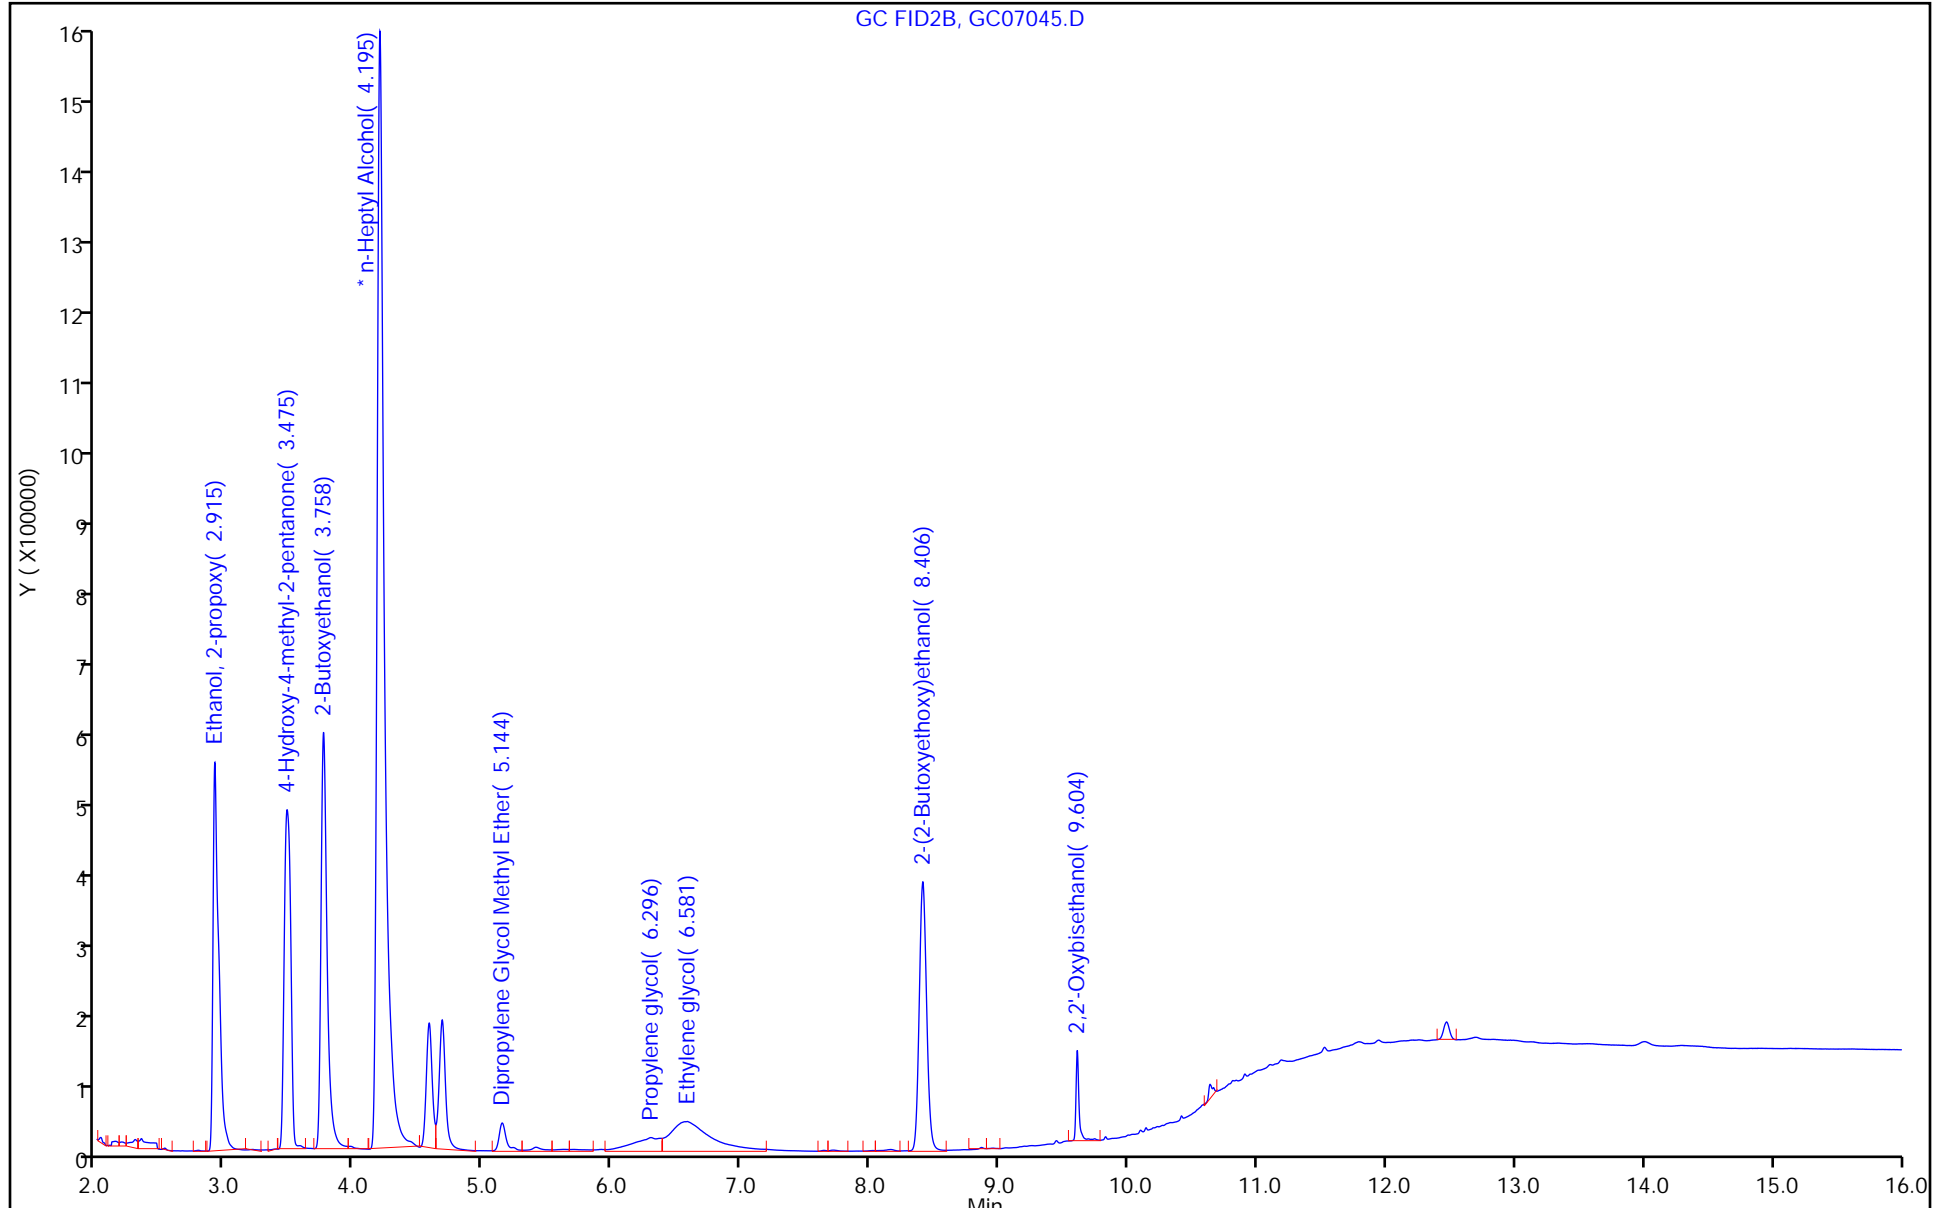

GC FID2B, GC07045.D

FORM I
GC SEMI VOA ORGANICS ANALYSIS DATA SHEET

Lab Name: Eurofins Savannah Job No.: 580-124266-1
SDG No.: _____
Client Sample ID: AF-RHMW02-WGN01LF-2302W4 Lab Sample ID: 580-124266-2 MSD
MSD
Matrix: Water Lab File ID: GC07046.D
Analysis Method: 8015C GLY Date Collected: 03/02/2023 11:10
Extraction Method: _____ Date Extracted: _____
Sample wt/vol: 1(mL) Date Analyzed: 03/08/2023 06:28
Con. Extract Vol.: 1(mL) Dilution Factor: 1
Injection Volume: 1(uL) GC Column: J&W DB WAX ID: 0.45(mm)
% Moisture: _____ % Solids: _____ GPC Cleanup: (Y/N) N
Cleanup Factor: _____
Analysis Batch No.: 766428 Units: mg/L

CAS NO.	COMPOUND NAME	RESULT	Q	LOQ	LOD	DL
112-34-5	2-(2-Butoxyethoxy)ethanol	28.2		5.0	3.0	1.1

Eurofins Savannah
Target Compound Quantitation Report

Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07046.D
 Lims ID: 580-124266-A-2 MSD
 Client ID:
 Sample Type: MSD
 Inject. Date: 08-Mar-2023 06:28:50 ALS Bottle#: 0 Worklist Smp#: 38
 Injection Vol: 1.0 ul Dil. Factor: 1.0000
 Sample Info: 680-0084239-038
 Operator ID: Instrument ID: CVGG2
 Method: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\8015_GLY_VGG.m
 Limit Group: 8015C_DAI
 Last Update: 08-Mar-2023 11:26:45 Calib Date: 07-Mar-2023 19:57:23
 Integrator: Falcon
 Quant Method: Internal Standard Quant By: Initial Calibration
 Last ICal File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07019.D
 Column 1 : J&W DB WAX (0.45 mm) Det: GC FID2B
 Process Host: CTX1619

First Level Reviewer: SWK1 Date: 08-Mar-2023 11:26:35

RT (min.)	Exp RT (min.)	Diff RT (min.)	Response	Cal Amt ug/ml	OnCol Amt ug/ml	Flags
1 Ethanol, 2-propoxy						
2.919	2.914	0.005	1750094	20.0	24.7	
2 4-Hydroxy-4-methyl-2-pentanone						
3.480	3.469	0.011	1799273	20.0	27.3	
3 2-Butoxyethanol						
3.760	3.758	0.002	1980695	20.0	24.2	
* 4 n-Heptyl Alcohol						
4.193	4.204	-0.011	6337151	50.0	50.0	
5 Dipropylene Glycol Methyl Ether						
5.148	5.136	0.012	159825	20.0	31.5	
6 Propylene glycol						
6.302	6.332	-0.030	251170	20.0	12.8	M
7 Ethylene glycol						
6.587	6.595	-0.008	1044833	20.0	21.0	
8 2-(2-Butoxyethoxy)ethanol						
8.406	8.407	-0.001	1639774	20.0	28.2	
9 2,2'-Oxybisethanol						
9.603	9.604	-0.001	291269	20.0	8.50	
10 Triethylene Glycol						
10.635	10.637	-0.002	66015	20.0	0.5913	7
LOD = 1.40						

QC Flag Legend

Processing Flags

7 - Failed Limit of Detection

Review Flags

M - Manually Integrated

Reagents:

SG_GlyICV_00055

Amount Added: 10.00

Units: uL

SG_GLY_ISTD_00106

Amount Added: 10.00

Units: uL

Run Reagent

Eurofins Savannah

Data File: \\chromfs\Savannah\ChromData\CVGG2\20230307-84239.b\GC07046.D

Injection Date: 08-Mar-2023 06:28:50

Instrument ID: CVGG2

Operator ID:

Lims ID: 580-124266-A-2 MSD

Worklist Smp#: 38

Client ID:

Injection Vol: 1.0 ul


Dil. Factor: 1.0000

ALS Bottle#: 0

Method: 8015_GLY_VGG

Limit Group: 8015C_DAI

Column: J&W DB WAX (0.45 mm)

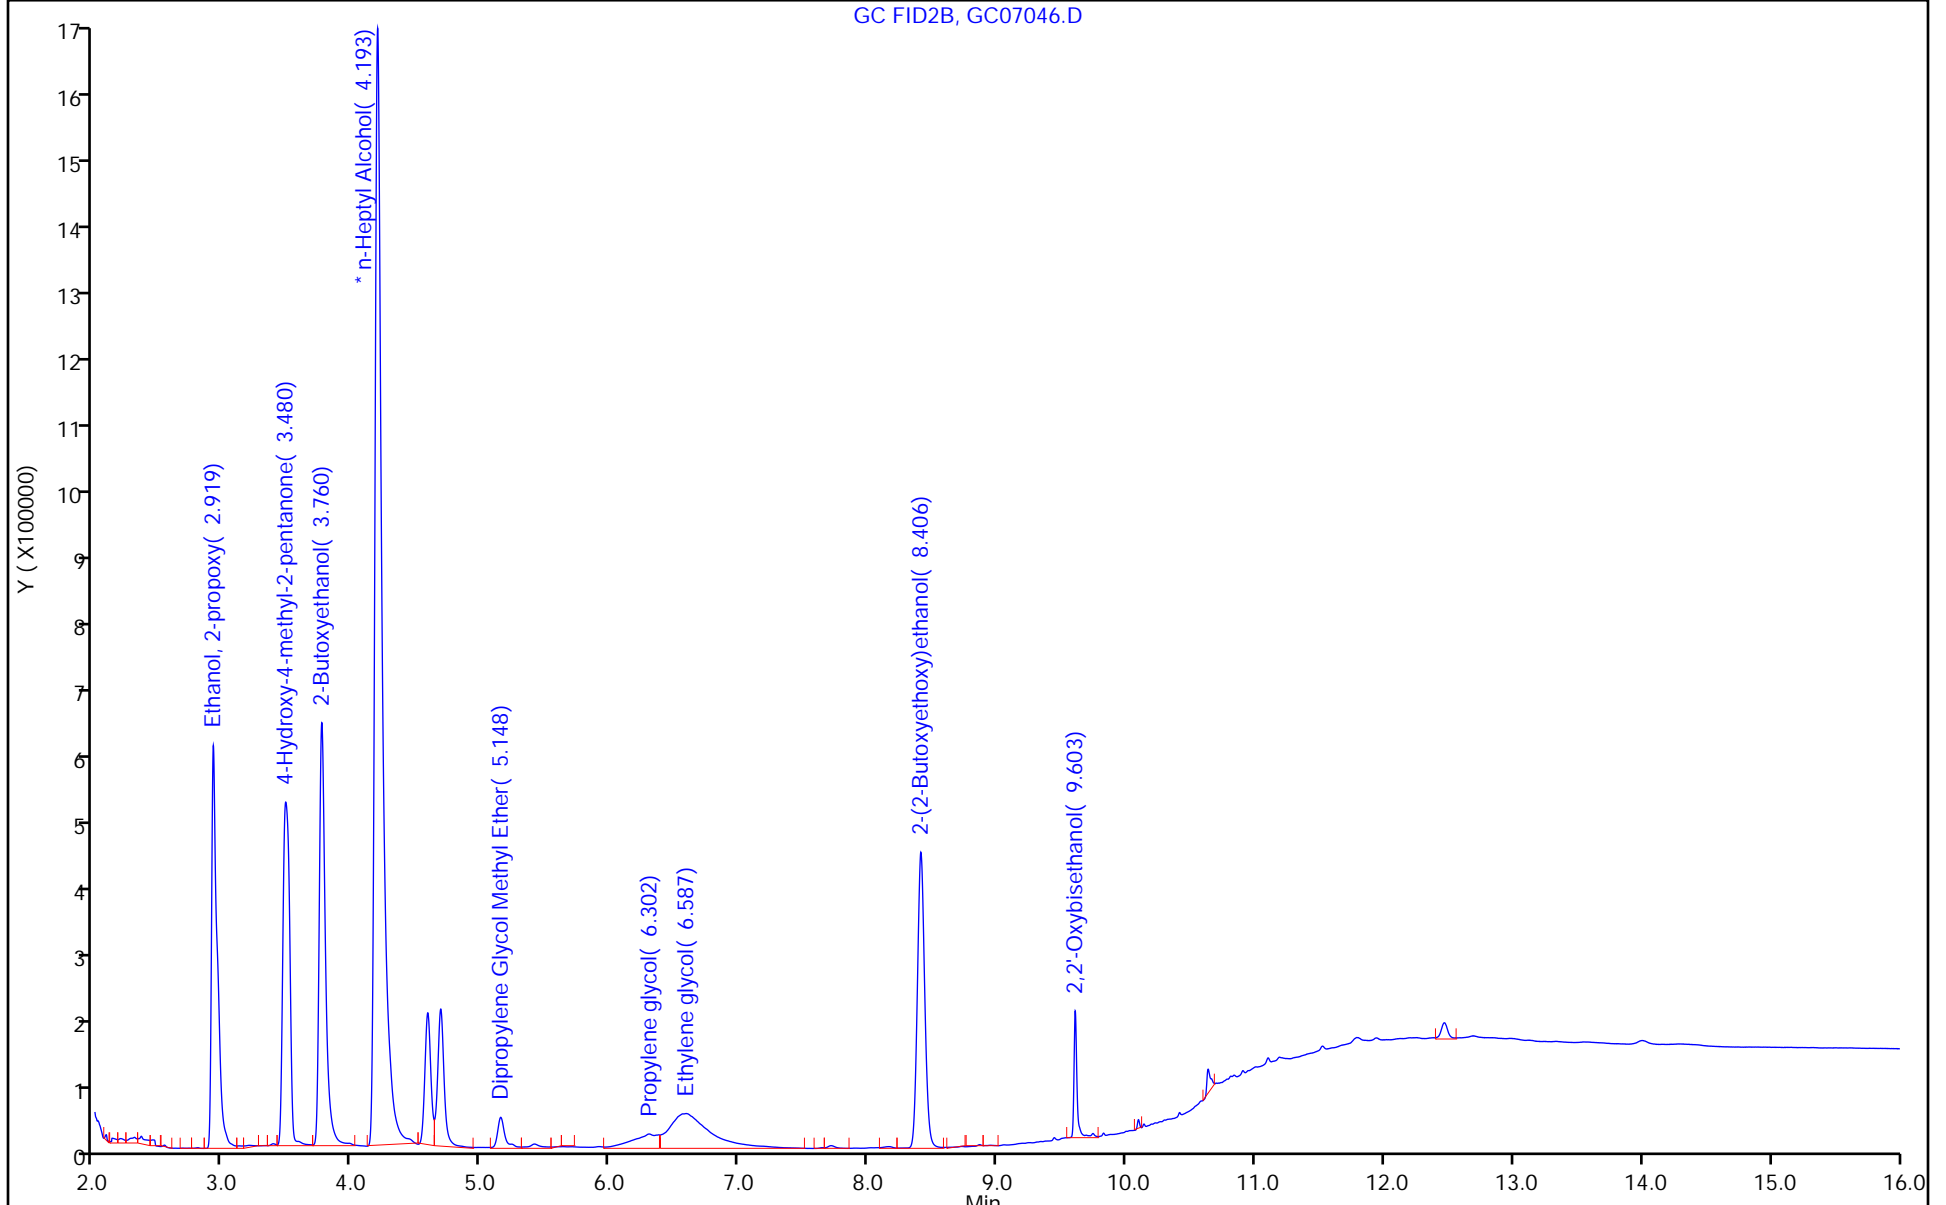

GC FID2B, GC07046.D

GC SEMI VOA ANALYSIS RUN LOG

Lab Name: Eurofins Savannah Job No.: 580-124266-1

SDG No.: _____

Instrument ID: CVGG2 Start Date: 03/07/2023 17:36

Analysis Batch Number: 766428 End Date: 03/08/2023 07:15

LAB SAMPLE ID	CLIENT SAMPLE ID	DATE ANALYZED	DILUTION FACTOR	LAB FILE ID	COLUMN ID
IC 680-766428/5		03/07/2023 17:36	1	GC07013.D	J&W DB WAX 0.45 (mm)
IC 680-766428/6		03/07/2023 18:00	1	GC07014.D	J&W DB WAX 0.45 (mm)
IC 680-766428/7		03/07/2023 18:23	1	GC07015.D	J&W DB WAX 0.45 (mm)
ICIS 680-766428/8		03/07/2023 18:46	1	GC07016.D	J&W DB WAX 0.45 (mm)
IC 680-766428/9		03/07/2023 19:10	1	GC07017.D	J&W DB WAX 0.45 (mm)
IC 680-766428/10		03/07/2023 19:33	1	GC07018.D	J&W DB WAX 0.45 (mm)
IC 680-766428/11		03/07/2023 19:57	1	GC07019.D	J&W DB WAX 0.45 (mm)
ICV 680-766428/12 CCV		03/07/2023 20:20	1	GC07020.D	J&W DB WAX 0.45 (mm)
LCS 680-766428/13		03/07/2023 20:44	1	GC07021.D	J&W DB WAX 0.45 (mm)
LCSD 680-766428/14		03/07/2023 21:07	1	GC07022.D	J&W DB WAX 0.45 (mm)
MB 680-766428/17		03/07/2023 22:18	1	GC07025.D	J&W DB WAX 0.45 (mm)
ZZZZZ		03/07/2023 22:41	10		J&W DB WAX 0.45 (mm)
ZZZZZ		03/07/2023 23:04	100		J&W DB WAX 0.45 (mm)
ZZZZZ		03/07/2023 23:28	1		J&W DB WAX 0.45 (mm)
ZZZZZ		03/07/2023 23:51	1		J&W DB WAX 0.45 (mm)
ZZZZZ		03/08/2023 00:15	1		J&W DB WAX 0.45 (mm)
ZZZZZ		03/08/2023 00:38	1		J&W DB WAX 0.45 (mm)
ZZZZZ		03/08/2023 01:02	1		J&W DB WAX 0.45 (mm)
ZZZZZ		03/08/2023 01:25	1		J&W DB WAX 0.45 (mm)
ZZZZZ		03/08/2023 01:48	1		J&W DB WAX 0.45 (mm)
ZZZZZ		03/08/2023 02:12	1		J&W DB WAX 0.45 (mm)
ZZZZZ		03/08/2023 02:35	1		J&W DB WAX 0.45 (mm)
ZZZZZ		03/08/2023 02:58	1		J&W DB WAX 0.45 (mm)
CCV 680-766428/32		03/08/2023 04:08	1	GC07040.D	J&W DB WAX 0.45 (mm)
580-124266-1	AF-RHMW03-WGN01LF-230 2W4	03/08/2023 05:18	1	GC07043.D	J&W DB WAX 0.45 (mm)
580-124266-2	AF-RHMW02-WGN01LF-230 2W4	03/08/2023 05:42	1	GC07044.D	J&W DB WAX 0.45 (mm)
580-124266-2 MS	AF-RHMW02-WGN01LF-230 2W4 MS	03/08/2023 06:05	1	GC07045.D	J&W DB WAX 0.45 (mm)
580-124266-2 MSD	AF-RHMW02-WGN01LF-230 2W4 MSD	03/08/2023 06:28	1	GC07046.D	J&W DB WAX 0.45 (mm)
CCV 680-766428/40		03/08/2023 07:15	1	GC07048.D	J&W DB WAX 0.45 (mm)

GC SEMI VOA BATCH WORKSHEET

Lab Name: Eurofins Savannah Job No.: 580-124266-1

SDG No.: _____

Batch Number: 766428 Batch Start Date: 03/07/23 17:36 Batch Analyst: Kellar, Joshua C

Batch Method: 8015C GLY Batch End Date: _____

Lab Sample ID	Client Sample ID	Method Chain	Basis	FinalAmount	SG_Gly_CAL 00048	SG_GLY_ISTD 00106	SG_GlyICV 00055		
IC 680-766428/5		8015C GLY		1 mL	50 uL	10 uL			
IC 680-766428/6		8015C GLY		1 mL	40 uL	10 uL			
IC 680-766428/7		8015C GLY		1 mL	25 uL	10 uL			
ICIS 680-766428/8		8015C GLY		1 mL	10 uL	10 uL			
IC 680-766428/9		8015C GLY		1 mL	5 uL	10 uL			
IC 680-766428/10		8015C GLY		1 mL	2.5 uL	10 uL			
IC 680-766428/11		8015C GLY		1 mL	1 uL	10 uL			
ICV 680-766428/12 CCV		8015C GLY		1 mL		10 uL	10 uL		
LCS 680-766428/13		8015C GLY		1 mL		10 uL	10 uL		
LCSD 680-766428/14		8015C GLY		1 mL		10 uL	10 uL		
MB 680-766428/17		8015C GLY		1 mL		10 uL			
CCV 680-766428/32		8015C GLY		1 mL	10 uL	10 uL			
580-124266-A-1	AF-RHMW03-WGN01L F-2302W4	8015C GLY	T	1 mL		10 uL			
580-124266-A-2	AF-RHMW02-WGN01L F-2302W4	8015C GLY	T	1 mL		10 uL			
580-124266-A-2	AF-RHMW02-WGN01L F-2302W4	8015C GLY	T	1 mL		10 uL	10 uL		
580-124266-A-2	AF-RHMW02-WGN01L F-2302W4	8015C GLY	T	1 mL		10 uL	10 uL		
MSD CCV 680-766428/40		8015C GLY		1 mL	10 uL	10 uL			

Batch Notes	

Basis	Basis Description
T	Total/NA

The pound sign (#) in the amount added field denotes that the reagent was used undiluted. All calculations are performed using the stated concentration for this reagent.


Subcontract Data

Shipping and Receiving Documents

Client Information Address: 1001 Bishop St, Suite 1600 City: Honolulu State, Zip: Hawaii 96813 Phone: 808-954-4512 / 770-331-0794 Email: Watson Tanji (watson.tanji@aeacom.com) / Mark Kromis (mark.kromis@aeacom.com) Project Name: CTO N6274223F0104 Site: RHSF		Sampler: <u>Matt Yim</u> Phone: <u>808-349-4737</u> PWSID: _____		Lab PIV: Elaine Walker E-Mail: M.Elaine.Walker@EurofinsET.com		Carrier Tracking No(s): FedEx State of Origin: Hawaii COC No: 2302W4FEA02 Page: Page 1 of 1 Job #: _____	
Due Date Requested: see subcontract TAT Requested (days): <u>Rush - ASAP</u> Compliance Project: <input type="checkbox"/> Yes <input type="checkbox"/> No PO #: _____ WO #: _____		Analysis Requested 8015C_DAI_GL_DS/2-(2-butoxyethoxy)-ethanol Perform MS/MSD (Yes or No) <input checked="" type="checkbox"/> A Field Filtered Sample (Yes or No) <input checked="" type="checkbox"/> N		Preservation Codes: A - HCl B - NaOH C - Zn Acetate D - Nitric Acid E - NaHSO4 F - MeOH G - Amchlor H - Ascorbic Acid I - Ice J - DI Water K - EDTA L - EDA Other: _____		Preservation Codes: M - Hexane N - None O - AsNaO2 P - Na2O4S Q - Na2SO3 R - Na2SO3 S - H2SO4 T - TSP Dodecahydrate U - Acetone V - MCAA W - pH 4-5 Z - other (specify)	
Sample Identification AF-RHMW03-WGN01LF-2302W4		Sample Date: 3/12/23 Sample Time: 1245 Sample Type (G=Comp, G=grab): G Matrix (Mineral, Swallow, Other): _____		Total Number of Containers: 3		Special Instructions/Note: _____	
Possible Hazard Identification <input checked="" type="checkbox"/> Non-Hazard <input type="checkbox"/> Flammable <input type="checkbox"/> Skin Irritant <input type="checkbox"/> Poison B <input type="checkbox"/> Unknown <input type="checkbox"/> Radiological		Sample Disposal (A fee may be assessed if samples are retained longer than 1 month) <input type="checkbox"/> Return To Client <input type="checkbox"/> Disposal By Lab <input type="checkbox"/> Archive For _____ Months		Total Number of Containers: 3		Special Instructions/Note: _____	
Deliverable Requested: I, II, III, IV, Other (specify) _____		Prelim data (Level 1 or 2) - see TAT above. DoD Stage 4 report standard. IAT_AECOM.EQUIS.EDD		Special Instructions/QC Requirements: DOD QSM project.		Method of Shipment: _____	
Empty Kit Relinquished by: _____		Relinquished by: <u>Matt Yim</u> Date: <u>3/12/23</u> Time: _____		Received by: <u>James Mason</u> Date/Time: <u>3/12/23 1400</u> Company: <u>AECOM</u>		Relinquished by: <u>James Mason</u> Date/Time: <u>3-9-23 900</u> Company: _____	
Relinquished by: <u>James Mason</u> Date/Time: <u>3/12/23 1415</u> Company: <u>AECOM</u>		Relinquished by: _____ Date/Time: _____ Company: _____		Relinquished by: _____ Date/Time: _____ Company: _____		Cooler Temperature(s) °C and Other Remarks: <u>5.9/5.9</u>	

Client Information Company: AECOM Address: 1001 Bishop St. Suite 1600 City: Honolulu State, Zip: Hawaii 96813 Phone: 808-954-4512 / 770-331-0794 Email: watson.tanji@aeocom.com / Mark Kromis (mark.kromis@aeocom.com) Project Name: CTO N6274223F0104 Site: RHSF		Lab PM: Elaine Walker E-Mail: M.Elaine.Walker@EurofinsET.com Carrier Tracking No(s): FedEx State of Origin: Hawaii Page: Page 1 of 1 Job #:	
Due Date Requested: see subcontract TAT Requested (days): Rush - ASAP Compliance Project: <input type="checkbox"/> Yes <input checked="" type="checkbox"/> No PO #: WO #: Project #: 60697810 SSOw#:		Analysis Requested Total Number of Containers: 3 Preservation Codes: A - HCL B - NaOH C - Zn Acetate D - Nitric Acid E - NaHSO4 F - MeOH G - Amchlor H - Ascorbic Acid I - Ice J - DI Water K - EDTA L - EDA Other:	
Sample Identification AF-RHMM02-WGN01LF-2302W4 Sample Date: 3/2/23 Sample Time: 1100 Sample Type (C=Comp, G=grab): G Matrix (Re-water, Seawater, Other (Fluor, Arsenic)):		Field Filtered Sample (Yes or No): Perform MS/MSD (Yes or No): 8015C_DAI_GL_DS/2-(2-butylethoxy)-ethanol A X N X N X Special Instructions/Note:	
Possible Hazard Identification <input checked="" type="checkbox"/> Non-Hazard <input type="checkbox"/> Flammable <input type="checkbox"/> Skin Irritant <input type="checkbox"/> Poison B <input type="checkbox"/> Radiological Deliverable Requested: I, II, III, IV, Other (specify) Empty Kit Relinquished by:			
Relinquished by: <i>Andy Young</i> Date/Time: 3/2/23 1400 Company: AECOM		Received by: James Mason Date/Time: 3/2/23 1400 Company: AECOM	
Relinquished by: James Mason Date/Time: 3/2/23 1415 Company: AECOM		Received by: <i>[Signature]</i> Date/Time: 3-4-23 900 Company:	
Relinquished by:		Received by:	
Custody Seals Intact: <input type="checkbox"/> Yes <input checked="" type="checkbox"/> No		Cooler Temperature(s) °C and Other Remarks: 5.9 / 5.9	

Chain of Custody Record



Environm. Testing
America

Client Information Company: AECOM Address: 1001 Bishop St. Suite 1600 City: Honolulu State: HI Zip: 96813 Phone: 808-954-4512 / 770-331-0794 Email: Watson.Tanji@aecom.com / Mark.Kromis@aecom.com Project Name: CTO N6274223F0104 Site: RHSF		Lab PM: Elaine Walker E-Mail: Elaine.Walker@EurofinsET.com Carrier Tracking No(s): FedEX State of Origin: Hawaii		COC No: 2302W4AFE02 Page: Page 1 of 1 Job #:		
Due Date Requested: see subcontract TAT Requested (days): Rush - ASAP Compliance Project: <input type="checkbox"/> Yes <input type="checkbox"/> No PO #: WO #: Project #: 60697810 SSO#:		Analysis Requested 8015C_DAI_GL_DS/2-(2-butoxyethoxy)-ethanol Perform MS/MSD (Yes or No) <input checked="" type="checkbox"/> A Field Filtered Sample (Yes or No) <input checked="" type="checkbox"/> N Total Number of Containers <input checked="" type="checkbox"/> 3				
Sample Identification AF-RHMW03-WGN01LF-2302W4		Sample Date 3/2/23	Sample Time 1245	Sample Type (C=Comp, G=grab) G	Matrix (Water, Soil, Organic/L, B/Tissue, As/Air) W	Preservation Code W
Possible Hazard Identification <input checked="" type="checkbox"/> Non-Hazard <input type="checkbox"/> Flammable <input type="checkbox"/> Skin Irritant <input type="checkbox"/> Poison B <input type="checkbox"/> Unknown <input type="checkbox"/> Radiological		Sample Disposal (A fee may be assessed if samples are retained longer than 1 month) <input type="checkbox"/> Return To Client <input checked="" type="checkbox"/> Disposal By Lab <input type="checkbox"/> Archive For _____ Months				
Deliverable Requested I II III IV Other (specify)		Prelim data (Level 1 or 2) - see TAT above DoD Stage 4 report standard TAT. AECOM EQUIS.EDD.				
Empty Kit Relinquished by		Method of Shipment:				
Relinquished by: Matt Jim Mathysen		Date: 3/2/23		Date/Time: 3/2/23 1400		
Relinquished by: James Mason		Date: 3/2/23		Date/Time: 3-4-23 900		
Relinquished by:		Date:		Date/Time:		
Custody Seals Intact: <input type="checkbox"/> Yes <input type="checkbox"/> No		Cooler Temperature(s) °C and Other Remarks: 5.9/5.9				

Chain of Custody Record

Client Information		Sampler: <u>Andy Young</u>		Lab PM: <u>Elaine Walker</u>		Carrier Tracking No(s): <u>FedEX</u>		IOC No: <u>2302W4FEA01</u>	
Client Contact:		Phone: <u>402-571-5712</u>		E-Mail: <u>M.Elaine.Walker@EurofinsET.com</u>		State of Origin: <u>Hawaii</u>		Page: <u>1 of 1</u>	
Company: <u>AECOM</u>		PWSID:		Analysis Requested		Analysis Requested		Job #: _____	
Address: <u>1001 Bishop St. Suite 1600</u>		Due Date Requested: <u>See subcontract</u>		Field Filtered Sample (Yes or No)		Perform MS/MSD (Yes or No)		Total Number of Containers: <u>3</u>	
City: <u>Honolulu</u>		TAT Requested (days): <u>Rush - ASAP</u>		Sample Date		Sample Time		Sample Type (C=Comp, G=grab)	
State, Zip: <u>Hawaii 96813</u>		Compliance Project: <u>Yes</u> <input type="checkbox"/> <u>No</u> <input type="checkbox"/>		Sample Date: <u>3/2/23</u>		Sample Time: <u>1100</u>		Sample Type: <u>G</u>	
Phone: <u>808-954-4512 / 770-331-0794</u>		PO #:		Preservation Code:		Matrix (W=Water, S=solid, O=swastical, A=Asst)		Special Instructions/Note:	
Email: <u>Watson.Tanji@aeom.com / Mark.Kromis@aeom.com</u>		WO #:		Sample Date: <u>3/2/23</u>		Sample Time: <u>1100</u>		Sample Type: <u>G</u>	
Project Name: <u>CTO N6274223F0104</u>		Project #:		Sample Date: <u>3/2/23</u>		Sample Time: <u>1100</u>		Sample Type: <u>G</u>	
Site: <u>RHSF</u>		SSOW#:		Sample Date: <u>3/2/23</u>		Sample Time: <u>1100</u>		Sample Type: <u>G</u>	
Sample Identification		Sample Date		Sample Time		Sample Type		Matrix	
<u>AF-RHMW02-WGN01LF-2302W4</u>		<u>3/2/23</u>		<u>1100</u>		<u>G</u>		<u>W</u>	
Possible Hazard Identification		Unknown <input type="checkbox"/>		Radiological <input type="checkbox"/>		Poison B <input type="checkbox"/>		Skin Irritant <input type="checkbox"/>	
Deliverable Requested: I, II, III, IV, Other (specify)		Flammable <input type="checkbox"/>		Non-Hazard <input type="checkbox"/>		Other (specify)		Other (specify)	
Empty Kit Relinquished by		Date		Date		Date		Date	
Relinquished by: <u>Andy Young ASG</u>		Date: <u>3/2/23</u>		Date: <u>1400</u>		Date: <u>3/2/23</u>		Date: <u>1400</u>	
Relinquished by: <u>James Mason</u>		Date: <u>3/2/23</u>		Date: <u>1415</u>		Date: <u>3/2/23</u>		Date: <u>900</u>	
Relinquished by:		Date:		Date:		Date:		Date:	
Custody Seals Intact: <u>Yes</u> <input type="checkbox"/> <u>No</u> <input type="checkbox"/>		Custody Seal No		Cooler Temperature(s) °C and Other Remarks: <u>5.9 / 5.9</u>		Company: <u>AECOM</u>		Company: <u>AECOM</u>	

Login Sample Receipt Checklist

Client: AECOM

Job Number: 580-124266-1

Login Number: 124266
List Number: 1
Creator: Presley, Kim A

List Source: Eurofins Seattle

Question	Answer	Comment
Radioactivity wasn't checked or is \leq background as measured by a survey meter.	N/A	
The cooler's custody seal, if present, is intact.	N/A	
Sample custody seals, if present, are intact.	N/A	
The cooler or samples do not appear to have been compromised or tampered with.	N/A	
Samples were received on ice.	True	
Cooler Temperature is acceptable.	True	
Cooler Temperature is recorded.	True	
COC is present.	True	
COC is filled out in ink and legible.	True	
COC is filled out with all pertinent information.	True	
Is the Field Sampler's name present on COC?	True	
There are no discrepancies between the containers received and the COC.	N/A	
Samples are received within Holding Time (excluding tests with immediate HTs)	True	
Sample containers have legible labels.	N/A	
Containers are not broken or leaking.	N/A	
Sample collection date/times are provided.	True	
Appropriate sample containers are used.	N/A	
Sample bottles are completely filled.	N/A	
Sample Preservation Verified.	N/A	
There is sufficient vol. for all requested analyses, incl. any requested MS/MSDs	N/A	
Containers requiring zero headspace have no headspace or bubble is $<6\text{mm}$ (1/4").	N/A	
Multiphasic samples are not present.	N/A	
Samples do not require splitting or compositing.	N/A	
Residual Chlorine Checked.	N/A	

Login Sample Receipt Checklist

Client: AECOM

Job Number: 580-124266-1

Login Number: 124266
List Number: 2
Creator: Meincke, Griffin E

List Source: Eurofins Savannah
List Creation: 03/07/23 01:20 PM

Question	Answer	Comment
Radioactivity wasn't checked or is \leq background as measured by a survey meter.		
The cooler's custody seal, if present, is intact.		
Sample custody seals, if present, are intact.		
The cooler or samples do not appear to have been compromised or tampered with.		
Samples were received on ice.		
Cooler Temperature is acceptable.		
Cooler Temperature is recorded.		
COC is present.		
COC is filled out in ink and legible.		
COC is filled out with all pertinent information.		
Is the Field Sampler's name present on COC?		
There are no discrepancies between the containers received and the COC.		
Samples are received within Holding Time (excluding tests with immediate HTs)		
Sample containers have legible labels.		
Containers are not broken or leaking.		
Sample collection date/times are provided.		
Appropriate sample containers are used.		
Sample bottles are completely filled.		
Sample Preservation Verified.		
There is sufficient vol. for all requested analyses, incl. any requested MS/MSDs		
Containers requiring zero headspace have no headspace or bubble is $<6\text{mm}$ (1/4").		
Multiphasic samples are not present.		
Samples do not require splitting or compositing.		
Residual Chlorine Checked.		