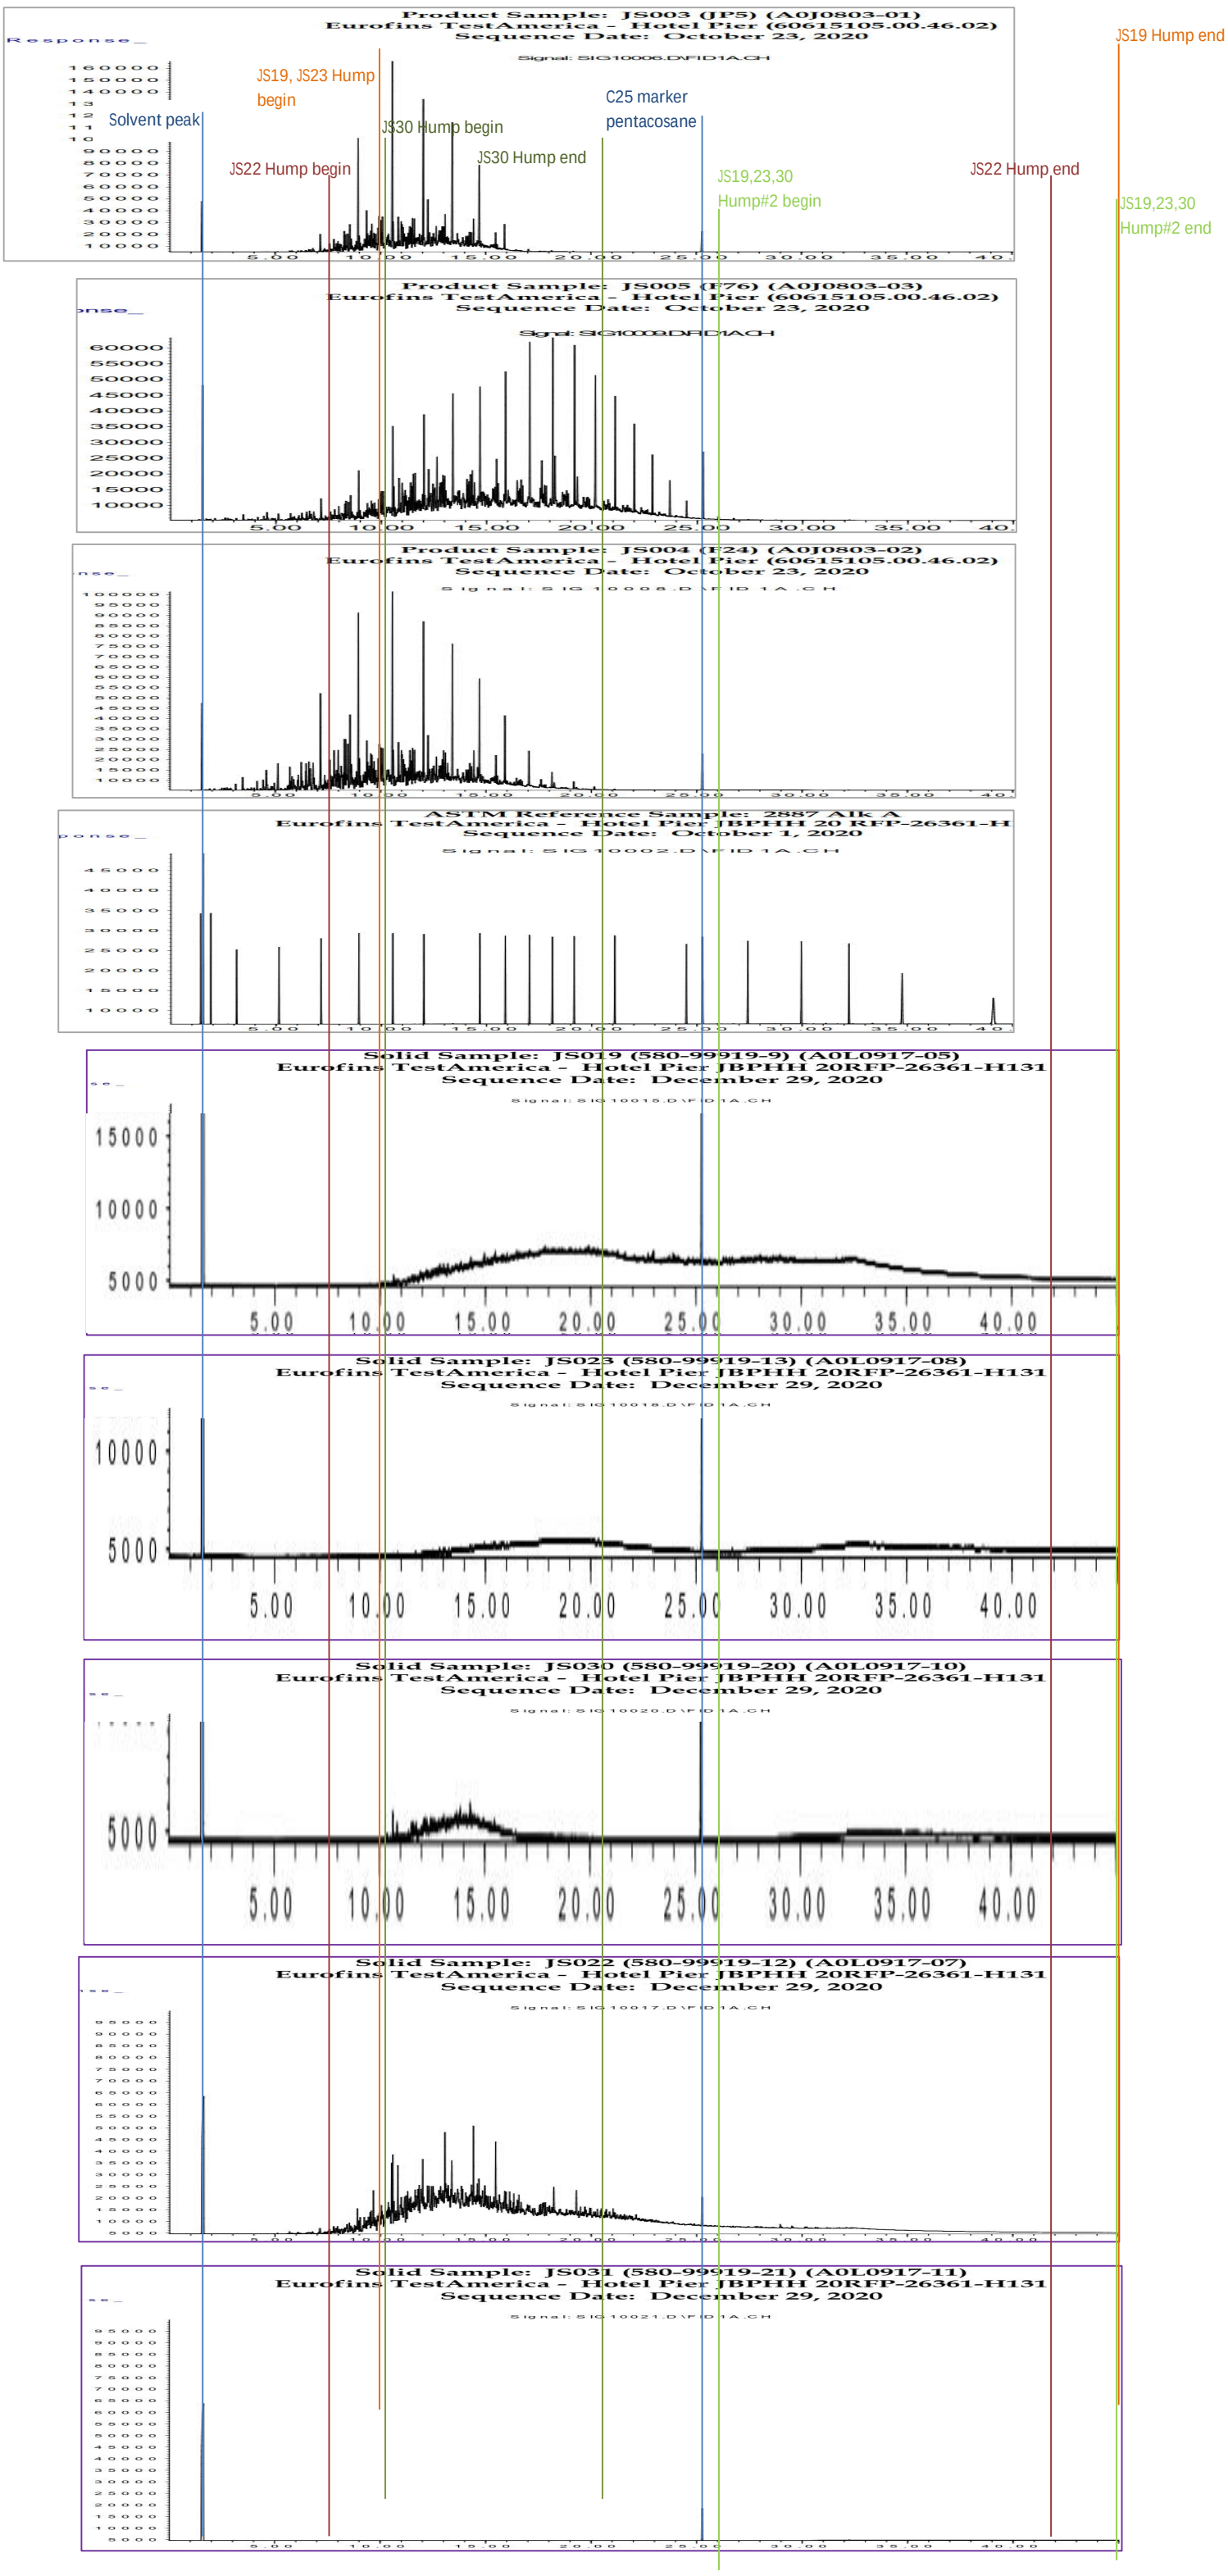
Product Sample: JS003 (JP5) (A0J0803-01)
Eurofins TestAmerica - Hotel Pier (60615105.00.46.02)
Sequence Date: October 23, 2020
Solvent peak
JS19, JS23 Hump begin
JS22 Hump begin
JS30 Hump begin
JS30 Hump end
C25 marker pentacosane
JS19,23,30 Hump#2 begin
JS22 Hump end
JS19 Hump end
JS19,23,30 Hump#2 end
Product Sample: JS005 (F76) (A0J0803-03)
Eurofins TestAmerica - Hotel Pier (60615105.00.46.02)
Sequence Date: October 23, 2020
Product Sample: JS004 (F24) (A0J0803-02)
Eurofins TestAmerica - Hotel Pier (60615105.00.46.02)
Sequence Date: October 23, 2020
ASTM Reference Sample: 2887 Alk A
Eurofins TestAmerica - Hotel Pier JBPHH 20 RFP-26361-H
Sequence Date: October 1, 2020
Solid Sample: JS019 (580-99919-9) (A0L0917-05)
Eurofins TestAmerica - Hotel Pier JBPHH 20RFP-26361-H131
Sequence Date: December 29, 2020
Solid Sample: JS023 (580-99919-13) (A0L0917-08)
Eurofins TestAmerica - Hotel Pier JBPHH 20RFP-26361-H131
Sequence Date: December 29, 2020
Solid Sample: JS030 (580-99919-20) (A0L0917-10)
Eurofins TestAmerica - Hotel Pier JBPHH 20RFP-26361-H131
Sequence Date: December 29, 2020
Solid Sample: JS022 (580-99919-12) (A0L0917-07)
Eurofins TestAmerica - Hotel Pier JBPHH 20RFP-26361-H131
Sequence Date: December 29, 2020
Solid Sample: JS031 (580-99919-21) (A0L0917-11)
Eurofins TestAmerica - Hotel Pier JBPHH 20RFP-26361-H131
Sequence Date: December 29, 2020