



908 North Temperance Ave. ▽ Clovis, CA 93611 ▽ Phone 559-275-2175 ▽ Fax 559-275-4422

Certification Number: CA1312
NELAP Certification number: CA00046
DoD-ELAP Certificate number: 4064.01

Data Validatable Report

November 30, 2021

AECOM
1001 Bishop Street, Suite 1600
Honolulu, Hawaii 96813

Attn: Alethea Ramos

Title: Report of Data: Case 97923

Project: 60571032 CV18F0126 Red Hill Fuel Storage, HI

Contract #: Prime contract # for DoD: NAVY CLEAN N62742-17-F-1800, CV18F0126
Subcontract: 18S-22209-HI27

Dear Ms. Ramos:

Two water samples were received October 21, 2021. Written results for the requested analyses are being provided on this November 30, 2021.

Results in this report apply to the samples analyzed in accordance with the chain of custody document. This analytical report must be reproduced in its entirety.

If you have any questions or require further information, please contact your APPL Project Manager, Libby Cheeseborough, libby@applinc.com, at your convenience. Thank you for choosing APPL, Inc.

I certify that this data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. These test results meet all requirements of NELAC and DoD QSM. Release of the hard copy has been authorized by the Laboratory Manager or his designee, as verified by the following signature.

Loren Portwood, Laboratory Director
APPL, Inc.

LP/lac
Enclosure
cc: File

Data Validation Package
for
60571032 CV18F0126 Red Hill Fuel Storage
APPL SDG 97923
TABLE OF CONTENTS

LABORATORY NAME: APPL, Inc.

Case Narrative	<u>3</u>
Sample Management Records	<u>7</u>
Sample Results	<u>12</u>
QC Forms	<u>19</u>
Method 8270D SIM Calibration Data	<u>48</u>
Method 8270D SIM Raw Data	<u>75</u>
Method 8260B Calibration Data	<u>96</u>
Method 8260B Raw Data	<u>157</u>
Method 8260B GRO Calibration Data	<u>181</u>
Method 8260B GRO Raw Data	<u>217</u>
Inorganic Analyses and Calibration Raw Data	<u>237</u>

CASE NARRATIVE

Case Narrative

ARF: 97923

Project: 60571032 CV18F0126 Red Hill Fuel Storage. HI

Sample Receipt Information:

Two water samples were received October 21, 2021 2.1°C. The sample group was assigned Analytical Request Form (ARF) number 97923.

Sample Preparation and Analysis Information:

For the EPA 8270D SIM analysis, the sample was extracted according to EPA method 3520C.

For the EPA 8260B analysis, the samples were purged according to EPA method 5030B.

For the EPA 9060 analysis, the sample was prepared according to the method.

Only the portion of the injection log relative to these samples is included. A full sequence log is available upon request. Measurement uncertainty can be reported upon request.

Analytical Exceptions, Deviations and Abnormalities.

None.

qryCOC_APPLCaseNarrativeReport

SDG	Received	Client ID	APPL ID	Collected DateTime	Matrix	Method	Method Description
97923	10/21/2021	ERH1835	BA43836	10/20/2021 8:55:00 AM	WATER	EPA 8260B	EPA 8260B BTEX WATER
97923	10/21/2021	ERH1835	BA43836	10/20/2021 8:55:00 AM	WATER	EPA 8260B	EPA 8260B GRO WATER
97923	10/21/2021	ERH1836	BA43837	10/20/2021 9:15:00 AM	WATER	EPA 8260B	EPA 8260B BTEX WATER
97923	10/21/2021	ERH1836	BA43837	10/20/2021 9:15:00 AM	WATER	EPA 8260B	EPA 8260B GRO WATER
97923	10/21/2021	ERH1836	BA43837	10/20/2021 9:15:00 AM	WATER	8270D-SIM	EPA 8270D SIM LIQ-LIQ
97923	10/21/2021	ERH1836	BA43837	10/20/2021 9:15:00 AM	WATER	SW846 9060A	9060A TOC

Abbreviations and Flags


FLAG	DESCRIPTION
#	Recovery or RPD outside control limits
*	Recovery or RPD outside control limits
B	Analyte detected in associated method blank
C1	Reason for correction: wrote incorrect response
C2	Reason for correction: calculated incorrectly
C3	Reason for correction: needs to be rechecked
C4	Reason for correction: data not usable
DO	Diluted out
E	Exceeds linear range
F	Estimated value
G1	Includes a wide range of hydrocarbons which does not match our gasoline standard
G10	Includes a match to hydrocarbon profiles within the range of mineral spirits
G11	Includes a match to hydrocarbon profiles within the range of JP-4
G12	Pattern does not match the gasoline standard; the carbon range for this sample is consistent with JP8
G13	Closely resembles the hydrocarbon profile of aviation gasoline
G14	Analyte concentration may be biased due to carry over
G2	Closely resembles the boiling point hydrocarbon profile consistent with weathered gasoline
G3	Includes higher boiling hydrocarbons
G4	Includes dominant peak(s) not indicative of petroleum hydrocarbons
G5	Is mainly dominant peak(s) not indicative of petroleum hydrocarbons
G6	Contains recognizable contaminant peak(s) which has been removed from quantitation
G7	Is mainly a match to hydrocarbons within the range of gasoline
G8	Closely resembles the boiling point hydrocarbon profile consistent with weathered gasoline
G9	Includes hydrocarbons within the range of kerosene
J	Estimated value
M	Matrix effect
MI1	Manual integration: integration does not follow baseline
MI2	Manual integration: non-target peak interference
MI3	Manual integration: to split a peak that was integrated as one peak by the computer
MI4	Manual integration: to integrate a split peak
MI5	Manual integration: the whole peak or part of the peak was not integrated
MI6	Manual integration: computer integrated wrong peak
MI7	Manual integration: other - explain
MDL	Method detection limit
ND	Not detected
NT	Non-target
Q	Acceptance criteria not met
T1 I	Includes wide range of hydrocarbons not indicative of diesel
T1 M	Is mainly wide range of hydrocarbons not necessarily indicative of diesel
T2 I	Includes lower boiling hydrocarbons, i.e. mineral spirits, kerosene, stoddard solvent, white gas
T2 M	Is mainly lower boiling hydrocarbons, i.e. mineral spirits, kerosene, stoddard solvent, white gas
T3 I	Includes higher boiling hydrocarbons, i.e. asphaltene, waster oil, motor oil, or weathered diesel fuel
T3 M	Is mainly higher boiling hydrocarbons, i.e. asphaltene, waster oil, motor oil, or weathered diesel fuel
T4 I	Includes dominant peak(s) not indicative of hydrocarbons
T4 M	Is mainly dominant peak(s) not indicative of hydrocarbons
T5	Contains recognizable contaminant peak(s) which has been removed from quantitation
T6	Is mainly a match to hydrocarbons within range of diesel fuel
T7	Closely resembles the boiling point hydrocarbon profile consistent with diesel fuel
T8	Includes a match to hydrocarbon profiles within range of diesel and kerosene fuel
T9 I	Includes non-diesel hydrocarbons within boiling point range of diesel fuel
T9 M	Is mainly non-diesel hydrocarbons within boiling point range of diesel fuel.
Y	Percent difference between primary and confirmation column > 40%

SAMPLE RECORDS MANAGEMENT
CHAIN OF CUSTODY,
ARF, CRF, AND
CLIENT COMMUNICATION

APPL - Analysis Request Form

97923

Client: AECOM
 Address: 1001 Bishop Street, Suite 1600
Honolulu, HI 96813
 Attn: Alethea Ramos
 Phone: 808-954-4536 Fax: 808-523-8950
 Job: 60571032 CV18F0126 Red Hill Fuel Storage
 PO #: 18S-22209-HI27 PO# 102604
 Chain of Custody (Y/N): Y # 50081
 RAD Screen (Y/N): Y pH (Y/N): Y
 Turn Around Type: 1 WEEK

Received by: MSA 
 Date Received: 10/21/21 Time: 09:50
 Delivered by: FEDEX
 Shuttle Custody Seals (Y/N): Y Time Zone: -10
 Chest Temp(s): 2.1°C
 Color: VFRG/Receiving
 Samples Chilled until Placed in Refrig/Freezer: Y
 Project Manager: Libby Cheesebor
 QC Report Type: DVP4DOD/EQUIS/HI
 Due Date: 10/28/21

Comments:

PM: login and F1s to Margie.Pascua@aecom.com & alethea.ramos@aecom.com
AN: INCLUDE STANDARD PREP SHEETS!!!!!!
AN: 7 day TAT for Form 1s; 21 day TAT for PKG STYLE 1; DOD v5.1; DOD Forms: LOD database
Report MS/MSD/DUPs when AECOM sample used
8270 SIM: 1-methylnaphthalene, 2-methylnaphthalene & naphthalene only
FR: email ftp info to Margie, alethea.ramos@aecom.com, Stella, trommelfanger@lab-data.com & jcanlas@la
EDD: AECOM EQUIS EDD 2.5.3 to alethea.ramos@, Margie.Pascua@aecom.com, jecklund@lab-data.com

Sample Distribution:

GC: 1-\$SIM53LIQ51
Extractions: 1- LIQ003
VOA: 2-\$86BTOTXDOD5W, 2-\$GASBL, 2-\$GRO86BW
Wetlab: 1-\$TOCW53
Other: 1-HOLD

Charges:

Invoice To:

ACCOUNTS PAYABLE
1001 Bishop Street, Ste 1600
USAPImaging@aecom.com
mary.basano@aecom.com

Client ID	APPL ID	Sampled	Analyses Requested
1. ERH1835	LCSD BA43836W 	10/20/21 08:55	\$86BTOTXDOD5W, \$GASBL, \$GRO86BW -- See Comments
2. ERH1836	LCSD BA43837W 	10/20/21 09:15	\$86BTOTXDOD5W, \$GASBL, \$GRO86BW, \$SIM53LIQ51, \$TOCW53 -- See Comments
3. ERH1836 BLANK	LCSD BA43838W 	10/20/21 09:15	HOLD -- See Comments


Note: All times, excluding sample collection times, are Pacific Time Zone unless noted otherwise. Collection times are in: -10 UTC

APPL Sample Receipt Form

ARF# 97923

Sample	Container Type	Count	p
BA43836	¹³ VOAs - HCL	4	NA
BA43837	¹³ VOAs - HCL	4	NA
	¹⁷ Amber Liter	2	NA
	³² Clear VOA - H2SO4	2	NA
BA43838	³⁹ Amber Liter, HCL prsvd	1	NA

Sample	Container Type	Count	p
--------	----------------	-------	---



APPL, Inc.
908 N Temperance Ave
Clovis, CA 93611

Phone: (559) 275-2175
Fax: (559) 275-4422

CHAIN OF CUSTODY RECORD

C.O.C. 50081 NIE

079129
1/1

Report to: PLEASE PRINT
Company Name: AECOM Phone: _____
Address: 1001 Bishop St., Suite 1600 Honolulu, HI 96813 Fax: _____
Attn: Alethea Ramos (808) 521-3051
Alethea.Ramos@aecom.com
Project Name/Number: 00571032.02.20.01 Sampler (Print) MM,KL

Invoice to: PLEASE PRINT
Company Name: _____ Phone: _____
Address: _____
Attn: _____
Accounts Payable
Email: USA/Imaging@aecom.com Fax: _____

Purchase Order Number	Sample Identification	Sampler (Signature)	Location	Date Collected	Time Collected	Time Zone	No. of Containers	Matrix			Analysis Requested/Method Number	Date Shipped: <u>1/12/21</u>
								Aq	Sed.	Soil		
102604	ERA1835	<i>[Signature]</i>	Twp Blank	10/20/21	0855	HST	4	X	X	X	BTEX by 8260 TPH-G by 8260 TPH-% 8015 TPH-% SGC 8015 PAH SMDA List MS 8260 MS 9060	Carrier: <u>FedEx</u>
	ERA1836		RHWNV2254-01	4	0915	h	10	X	X	X		Waybill No.: _____ Comments: <u>Note: NIE - Log in separate form other COC</u>

Turnaround Requested: Standard 2-3 wk One week 24/48 Hrs. Other _____
Sample Disposal: Return to client Disposal by Lab (30-day retention)
Relinquished by sampler: REU Date: 10/21/21 Time: 15:00
Relinquished by: _____ Date: _____ Time: _____
Received at lab by: [Signature]
White: Return to client with report Yellow: Laboratory Copy Pink: Sampler See reverse side for Container Preservative and Sampling Information

[Handwritten notes: 1-methoxy naphthalene, 2-methoxy naphthalene, *Naphthalene, TPH-% and PAHs used, liquid-liquid extraction, methoxy naphthalene]

COOLER RECEIPT FORM

ARF: 97923

- 1) Project: 60571032 CV18F0126 Red Hill Fuel Storage Date Received: 10/21/2021
- 2) Coolers: Number of Coolers: 1
- 3) YES Were custody seals present and intact?
How many? 2 Name/Date on seal? SEE BELOW
- 4) YES Was there a shipping slip? Carrier name: FEDEX
- 5) Type of packing in cooler: bubble wrap popcorn foam plastic bags other
 wet ice dry ice no ice gel ice
- 6) YES Were cooler temperatures acceptable?
- 7) Serial number of calibrated thermometer used: R3 CF: -1.9°C
- 8) Cooler temp(s): In °C. Thermometer Temp / Corrected Temp
1: 4.0/2.1 2: _____ 3: _____ 4: _____ 5: _____ 6: _____
7: _____ 8: _____ 9: _____ 10: _____ 11: _____ 12: _____

Chain of custody:

- 9) YES Was a chain of custody received?
- 10) YES Were the custody papers complete/signed in the appropriate places?

Sample Labels:

- 11) YES Were all sample labels complete (sample ID, date/time of sampling, etc.)?
- 12) YES ~~NO~~ Did all container labels agree with custody papers?

Sample Containers:

- 13) YES Were all containers sealed in separate bags?
- 14) YES Did all containers arrive in good condition:(unbroken, no leakage, no cracked/broken lids)?
- 15) NO ~~YES~~ Were correct containers and preservatives used for the tests indicated?
- 16) YES Was a sufficient amount of sample sent for tests indicated?
- 17) No Were bubbles present in volatile samples?

If yes, the following were received with air bubbles:

Larger than a pea: _____

Smaller than a pea: _____


Preservation Hold time:

- 18) Yes Was a sufficient amount of holding time remaining to analyze the samples?
- 19) NA ~~Yes~~ Was the pH taken of all non-VOA preserved samples and written on the sample container?
- 20) NA ~~Yes~~ Was the pH of acid preserved non-VOA samples < 2?
- 21) NA Was the pH of the "basic" preserved samples for Cyanide > 12, Sulfide >9, Hexchrom >9?
- 22) NO Were unpreserved VOA Vials received for VOA Dept analysis?
- 23) NA If "yes", are the unpreserved VOA vials noted in the ADD TEST FIELD on the ARF?

pH strip lot number: ~~HC020115~~

Lab notified if pH was not adequate: _____

Notes/Deficiencies:

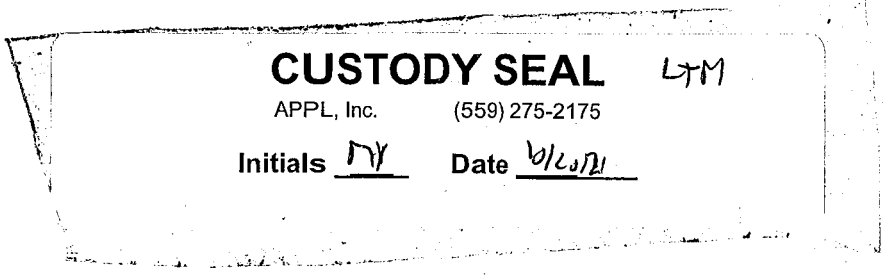

Did not receive any HCL preserved ampers for 8015 TPH analysis.

Personnel receiving samples: MS Second reviewer: MS
 Personnel labeling samples: DR
 Project manager notified: MS Date/Time of notification 10/21/2021
 Name of client notified: _____ Date/Time of notification _____

SAMPLE RESULTS

EPA 8270D SIM LIQ-LIQ

AECOM
1001 Bishop Street, Suite 1600
Honolulu, HI 96813

APPL Inc.
908 North Temperance Avenue
Clovis, CA 93611

Attn: Alethea Ramos

Project: 60571032 CV18F0126 Red Hill Fuel Storage

ARF: 97923

Sample ID: ERH1836

APPL ID: BA43837

Sample Collection Date: 10/20/21

QCG: #SIM53-211022A-270140

Method	Analyte	Result	LOQ	LOD	DL	Units	Extraction Date	Analysis Date
8270D-SIM	1-METHYLNAPHTHALENE	0.10 U	0.2	0.10	0.04	ug/L	10/22/21	10/28/21
8270D-SIM	2-METHYLNAPHTHALENE	0.10 U	0.2	0.10	0.04	ug/L	10/22/21	10/28/21
8270D-SIM	NAPHTHALENE	0.10 U	0.2	0.10	0.04	ug/L	10/22/21	10/28/21
8270D-SIM	SURROGATE: 2-METHYLNAPHTHALEN	78.2	39-114			%	10/22/21	10/28/21
8270D-SIM	SURROGATE: FLUORANTHENE-D10 (S	80.4	58-120			%	10/22/21	10/28/21

Quant Method: K1019.M
Run #: 1019K178
Instrument: KYLO
Sequence: 211019
Dilution Factor: 1
Initials: MA

Printed: 11/9/2021 9:26:43 AM
APPL-F1-SC-NoMC-REG MDLs-DOD

EPA 8260B BTEX WATER

AECOM
1001 Bishop Street, Suite 1600
Honolulu, HI 96813

Attn: Alethea Ramos
Project: 60571032 CV18F0126 Red Hill Fuel Storage

Sample ID: ERH1835

Sample Collection Date: 10/20/21

APPL Inc.
908 North Temperance Avenue
Clovis, CA 93611

ARF: 97923

APPL ID: BA43836

QCG: #86BTO-211026BM-269592

Method	Analyte	Result	LOQ	LOD	DL	Units	Extraction Date	Analysis Date
EPA 8260B	BENZENE	0.30 U	1.0	0.30	0.15	ug/L	10/27/21	10/27/21
EPA 8260B	ETHYLBENZENE	0.50 U	1.0	0.50	0.23	ug/L	10/27/21	10/27/21
EPA 8260B	TOLUENE	0.30 U	1.0	0.30	0.15	ug/L	10/27/21	10/27/21
EPA 8260B	XYLENES (TOTAL)	0.30 U	2.0	0.30	0.15	ug/L	10/27/21	10/27/21
EPA 8260B	SURROGATE: 1,2-DICHLOROETHANE-	100	81-118			%	10/27/21	10/27/21
EPA 8260B	SURROGATE: 4-BROMOFLUOROBENZ	96.9	85-114			%	10/27/21	10/27/21
EPA 8260B	SURROGATE: DIBROMOFLUOROMETH	104	80-119			%	10/27/21	10/27/21
EPA 8260B	SURROGATE: TOLUENE-D8 (S)	100.0	89-112			%	10/27/21	10/27/21

Quant Method: M1015W.M
Run #: 1026M35
Instrument: Max
Sequence: 211015
Dilution Factor: 1
Initials: PAN

Printed: 10/29/2021 4:56:00 AM
APPL-F1-SC-NoMC-REG MDLs-DOD

EPA 8260B BTEX WATER

AECOM
1001 Bishop Street, Suite 1600
Honolulu, HI 96813

Attn: Alethea Ramos
Project: 60571032 CV18F0126 Red Hill Fuel Storage

Sample ID: ERH1836

Sample Collection Date: 10/20/21

APPL Inc.
908 North Temperance Avenue
Clovis, CA 93611

ARF: 97923

APPL ID: BA43837

QCG: #86BTO-211026BM-269592

Method	Analyte	Result	LOQ	LOD	DL	Units	Extraction Date	Analysis Date
EPA 8260B	BENZENE	0.30 U	1.0	0.30	0.15	ug/L	10/27/21	10/27/21
EPA 8260B	ETHYLBENZENE	0.50 U	1.0	0.50	0.23	ug/L	10/27/21	10/27/21
EPA 8260B	TOLUENE	0.30 U	1.0	0.30	0.15	ug/L	10/27/21	10/27/21
EPA 8260B	XYLENES (TOTAL)	0.30 U	2.0	0.30	0.15	ug/L	10/27/21	10/27/21
EPA 8260B	SURROGATE: 1,2-DICHLOROETHANE-	97.2	81-118			%	10/27/21	10/27/21
EPA 8260B	SURROGATE: 4-BROMOFLUOROBENZ	96.1	85-114			%	10/27/21	10/27/21
EPA 8260B	SURROGATE: DIBROMOFLUOROMETH	101	80-119			%	10/27/21	10/27/21
EPA 8260B	SURROGATE: TOLUENE-D8 (S)	102	89-112			%	10/27/21	10/27/21

Quant Method: M1015W.M
Run #: 1026M36
Instrument: Max
Sequence: 211015
Dilution Factor: 1
Initials: PAN

Printed: 10/29/2021 4:56:00 AM
APPL-F1-SC-NoMC-REG MDLs-DOD

EPA 8260B GRO WATER

AECOM
1001 Bishop Street, Suite 1600
Honolulu, HI 96813

Attn: Alethea Ramos
Project: 60571032 CV18F0126 Red Hill Fuel Storage

Sample ID: ERH1835

Sample Collection Date: 10/20/21

APPL Inc.
908 North Temperance Avenue
Clovis, CA 93611

ARF: 97923

APPL ID: BA43836

QCG: #GRO86-211026BM-269634

Method	Analyte	Result	LOQ	LOD	DL	Units	Extraction Date	Analysis Date
EPA 8260B	GASOLINE RANGE ORGANICS	18.0 U	20	18.0	8.6	ug/L	10/27/21	10/27/21
EPA 8260B	SURROGATE: 4-BROMOFLUOROBENZ	98.3	85-114			%	10/27/21	10/27/21

Quant Method: M0825SUR.M
Run #: 1026M35
Instrument: Max
Sequence: 211015
Dilution Factor: 1
Initials: DA

Printed: 11/30/2021 1:30:40 PM
APPL-F1-SC-NoMC-REG MDLs-DOD

EPA 8260B GRO WATER

AECOM
1001 Bishop Street, Suite 1600
Honolulu, HI 96813

Attn: Alethea Ramos
Project: 60571032 CV18F0126 Red Hill Fuel Storage

Sample ID: ERH1836

Sample Collection Date: 10/20/21

APPL Inc.
908 North Temperance Avenue
Clovis, CA 93611

ARF: 97923

APPL ID: BA43837

QCG: #GRO86-211026BM-269634

Method	Analyte	Result	LOQ	LOD	DL	Units	Extraction Date	Analysis Date
EPA 8260B	GASOLINE RANGE ORGANICS	18.0 U	20	18.0	8.6	ug/L	10/27/21	10/27/21
EPA 8260B	SURROGATE: 4-BROMOFLUOROBENZ	97.5	85-114			%	10/27/21	10/27/21

Quant Method: M0825SUR.M
Run #: 1026M36
Instrument: Max
Sequence: 211015
Dilution Factor: 1
Initials: DA

Printed: 11/30/2021 1:30:40 PM
APPL-F1-SC-NoMC-REG MDLs-DOD

Wet Lab Analysis

AECOM
1001 Bishop Street, Suite 1600
Honolulu, HI 96813

APPL Inc.
908 North Temperance Avenue
Clovis, CA 93611

Attn: Alethea Ramos

Project: 60571032 CV18F0126 Red Hill Fuel Storage

Sample ID: ERH1836

Sample Collection Date: 10/20/2021

APPL ID: BA43837

ARF: 97923

Method	Analyte	Result	LOQ	LOD	DL	Units	DF	Prep Date	Analysis Date
SW846 9060A	TOTAL ORGANIC CARBON	0.18 J	0.93	0.350	0.130	mg/L	1	10/28/21	10/28/21

J = Estimated value.

Printed: 11/11/2021 1:44:03 PM

APPL-F1-SC-NoMC-REG MDLs

QC FORMS

8270D-SIM

Form 2 & 8

Surrogate Recovery

Lab Name: APPL, Inc.

SDG No: 97923

Case No: 97923

Date Analyzed: 10/28/2021

Matrix: WATER

Instrument: KYLO

APPL ID.	Client Sample No.	SURROGATE: 2-METHYLNAPHTHALENE-D10 (S)			SURROGATE: FLUORANTHENE-D10 (S)		
		Limits	Result	Qualifier	Limits	Result	Qualifier
211022A-BLK	Blank	39-114	77.3		58-120	82.5	
211022A-LCS	Lab Control Spike	39-114	84.4		58-120	88.2	
211022A-LCSD	Lab Control SpikeD	39-114	89.6		58-120	92.2	
BA43837	ERH1836	39-114	78.2		58-120	80.4	

Comments: Batch: #SIM53-211022A

Printed: 11/9/2021 9:26:37 AM
Form 2 & 8, Surrogate Recovery Summary

8270D-SIM

Form 4

Blank Summary

Lab Name: APPL, Inc.
Case No: 97923
Matrix: WATER
Blank ID: 211022A-BLK

SDG No: 97923
Date Analyzed: 10/28/2021
Instrument: KYLO
Time Analyzed: 0956

APPL ID.	Client Sample No.	File ID.	Date Analyzed
211022A-BLK	Blank	1019K172	10/28/2021 0956
211022A-LCS	Lab Control Spike	1019K173	10/28/2021 1016
211022A-LCSD	Lab Control Spiked	1019K174	10/28/2021 1036
BA43837	ERH1836	1019K178	10/28/2021 1155

Comments: Batch: #SIM53-211022A

Printed: 11/9/2021 9:26:31 AM
Form 4, Blank Summary

Method Blank
EPA 8270D SIM LIQ-LIQ

Blank Name/QCG: **211022W-43555 - 270140**
Batch ID: #SIM53-211022A

APPL Inc.
908 North Temperance Avenue
Clovis, CA 93611

Sample Type	Analyte	Result	LOQ	LOD	DL	Units	Extraction Date	Analysis Date
BLANK	1-METHYLNAPHTHALENE	0.10 U	0.2	0.10	0.04	ug/L	10/22/2021	10/28/2021
BLANK	2-METHYLNAPHTHALENE	0.10 U	0.2	0.10	0.04	ug/L	10/22/2021	10/28/2021
BLANK	NAPHTHALENE	0.10 U	0.2	0.10	0.04	ug/L	10/22/2021	10/28/2021
BLANK	SURROGATE: 2-METHYLNAPHT	77.3	39-114			%	10/22/2021	10/28/2021
BLANK	SURROGATE: FLUORANTHENE-	82.5	58-120			%	10/22/2021	10/28/2021

Quant Method: K1019.M
Run #: 1019K172
Instrument: KYLO
Sequence: 211019
Initials: MA

GC SC-Blank-REG MDLs-DOD
Printed: 11/9/2021 9:20:12 AM

8270D-SIM

Form 4

LCS Summary

Lab Name: APPL, Inc.
Case No: 97923
Matrix: WATER
LCS ID: 211022A-LCS

SDG No: 97923
Date Analyzed: 10/28/2021
Instrument: KYLO
Time Analyzed: 1016

APPL ID.	Client Sample No.	File ID.	Date Analyzed
211022A-BLK	Blank	1019K172	10/28/2021 0956
211022A-LCS	Lab Control Spike	1019K173	10/28/2021 1016
211022A-LCSD	Lab Control Spiked	1019K174	10/28/2021 1036
BA43837	ERH1836	1019K178	10/28/2021 1155

Comments: Batch: #SIM53-211022A

Laboratory Control Spike Recoveries

EPA 8270D SIM LIQ-LIQ

APPL ID: 211022W-43555 LCS - 270140

Batch ID: #SIM53-211022A

APPL Inc.

908 North Temperance Avenue

Clovis, CA 93611

Compound Name	Spike Lvl ug/L	SPK Result ug/L	DUP Result ug/L	SPK % Recovery	DUP % Recovery	Recovery Limits	RPD %	RPD Limits
1-METHYLNAPHTHALENE	5.00	4.23	4.64	84.6	92.8	41-115	9.2	20
2-METHYLNAPHTHALENE	5.00	4.27	4.74	85.4	94.8	39-114	10.4	20
NAPHTHALENE	5.00	4.12	4.56	82.4	91.2	43-114	10.1	20
<hr/>								
SURROGATE: 2-METHYLNAPHTHALEN	5.00	4.22	4.48	84.4	89.6	39-114		
SURROGATE: FLUORANTHENE-D10 (S)	5.00	4.41	4.61	88.2	92.2	58-120		

Comments: _____

<u>Primary</u>	<u>SPK</u>	<u>DUP</u>
Quant Method :	K1019.M	K1019.M
Extraction Date :	10/22/2021	10/22/2021
Analysis Date :	10/28/2021	10/28/2021
Instrument :	KYLO	KYLO
Run :	1019K173	1019K174
Initials :	MA	

Form 5
Tune Summary

Lab Name: APPL Inc.
 Case No: _____
 Matrix: Water
 ID: 1019K001.D

SDG No: _____
 Date Analyzed: 10/19/2021
 Instrument: KYLO
 Time Analyzed: 13:58

Client Sample No.	APPL ID.	File ID.	Date Analyzed
1	0.1 ug/ml 10/10/21	1019K002.D	10/19/2021 14:09
2	0.2 ug/ml 10/10/21	1019K003.D	10/19/2021 14:29
3	0.5 ug/ml 10/10/21	1019K004.D	10/19/2021 14:49
4	1 ug/ml 10/10/21	1019K005.D	10/19/2021 15:09
5	5 ug/ml 10/10/21	1019K006.D	10/19/2021 15:29
6	10 ug/ml 10/10/21	1019K007.D	10/19/2021 15:49
7	50 ug/ml 10/10/21	1019K008.D	10/19/2021 16:09
8	100 ug/ml 10/10/21	1019K009.D	10/19/2021 16:29
9	SS ug/ml 10/10/21	1019K010.D	10/19/2021 16:49
10			
11			
12			
13			
14			
15			
16			
17			
18			
19			
20			
21			
22			

m/e

51 9.95 - 80.1% of mass 198	<u>36.8</u>
68 0 - 2.05% of mass 69	<u>1.7</u>
70 0 - 2% of mass 69	<u>0.4</u>
127 10 - 80% of mass 198	<u>54.6</u>
197 0 - 2% of mass 198	<u>0.2</u>
198 100 - 100% of mass 198	<u>100.0</u>
199 5 - 9% of mass 198	<u>6.5</u>
275 10 - 60% of mass 198	<u>23.2</u>
365 1 - 100% of mass 198	<u>2.5</u>
441 0.01 - 24% of mass 442	<u>13.9</u>
442 50 - 500% of mass 198	<u>73.4</u>
443 15 - 24% of mass 442	<u>18.4</u>

Form 5
Tune Summary

Lab Name: APPL Inc.
Case No: 97923
Matrix: Water
ID: 1019K170.D

SDG No: 97923
Date Analyzed: 10/28/2021
Instrument: KYLO
Time Analyzed: 9:06

Client Sample No.	APPL ID.	File ID.	Date Analyzed
1	5 ug/ml 10/19/21 (1)	1019K171.D	10/28/2021 9:18
2	Blank	211021A BLK 1/1000	1019K172.D
3	Lab Control Spike	211021A LCS-1 1/1000	1019K173.D
4	Lab Control SpikeD	211021A LCSD-1 1/100	1019K174.D
5	ERH1836	BA43837W07 1/1000	1019K178.D
6	5 ug/ml 10/10/21 (2)	1019K205.D	10/28/2021 20:55
7			
8			
9			
10			
11			
12			
13			
14			
15			
16			
17			
18			
19			
20			
21			
22			

m/e

51 9.95 - 80.1% of mass 198	<u>30.6</u>
68 0 - 2.05% of mass 69	<u>1.5</u>
70 0 - 2% of mass 69	<u>0.5</u>
127 10 - 80% of mass 198	<u>51.2</u>
197 0 - 2% of mass 198	<u>0.3</u>
198 100 - 100% of mass 198	<u>100.0</u>
199 5 - 9% of mass 198	<u>6.6</u>
275 10 - 60% of mass 198	<u>23.5</u>
365 1 - 100% of mass 198	<u>2.5</u>
441 0.01 - 24% of mass 442	<u>13.7</u>
442 50 - 500% of mass 198	<u>80.0</u>
443 15 - 24% of mass 442	<u>18.8</u>

8A
INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: APPL Inc. Contract: _____
 Lab Code: _____ SDG No.: _____
 Lab File ID (Standard): 1019K171.D Date Analyzed: 10/28/21
 Instrument ID: KYLO Time Analyzed: 9:18
 GC Column: _____ ID: _____ Heated Purge: (Y/N) _____

		Napthalene-D8(IS)		Acenaphthene-D10(IS)		Phenanthrene-D10(IS)	
		AREA #	RT #	AREA #	RT #	AREA #	RT #
	12 HOUR STD	13064	3.89	6432	5.82	9841	7.52
	UPPER LIMIT	26128	4.06	12864	5.99	19682	7.69
	LOWER LIMIT	6532	3.72	3216	5.65	4921	7.35
	SAMPLE NO.						
01	211021A BLK 1/1000	12905	3.89	6299	5.82	9803	7.53
02	211021A LCS-1 1/1000	13479	3.89	6711	5.82	10307	7.52
03	211021A LCSD-1 1/1000	13301	3.89	6681	5.82	10357	7.52
04	BA43837W07 1/1000	13701	3.89	6820	5.82	10379	7.52
05	5 ug/ml 10/10/21 (2)	17438	3.89	8754	5.82	13434	7.52
06							
07							
08							
09							
10							
11							
12							
13							
14							
15							
16							
17							
18							
19							
20							
21							
22							

AREA UPPER LIMIT = +100% of internal standard area.
 AREA LOWER LIMIT = -50% of internal standard area.
 RT UPPER LIMIT = +0.17 minutes of internal standard RT
 RT LOWER LIMIT = -0.17 minutes of internal standard RT

Column used to flag values outside QC limits with an asterisk.
 * Values outside of QC limits.

8A
INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: APPL Inc. Contract: _____
 Lab Code: _____ SDG No.: _____
 Lab File ID (Standard): 1019K171.D Date Analyzed: 10/28/21
 Instrument ID: KYLO Time Analyzed: 9:18
 GC Column: _____ ID: _____ Heated Purge: (Y/N) _____

		Chrysene-D12(IS)		Perylene-D12(IS)			
		AREA	#	RT	#	AREA	#
	12 HOUR STD	11899		10.58		10623	12.76
	UPPER LIMIT	23798		10.75		21246	12.93
	LOWER LIMIT	5950		10.41		5312	12.59
	SAMPLE NO.						
01	211021A BLK 1/1000	11444		10.59		10357	12.76
02	211021A LCS-1 1/1000	12396		10.57		11238	12.76
03	211021A LCSD-1 1/1000	12395		10.57		11334	12.75
04	BA43837W07 1/1000	12461		10.57		10884	12.76
05	5 ug/ml 10/10/21 (2)	16058		10.57		14486	12.76
06							
07							
08							
09							
10							
11							
12							
13							
14							
15							
16							
17							
18							
19							
20							
21							
22							

AREA UPPER LIMIT = +100% of internal standard area.
 AREA LOWER LIMIT = -50% of internal standard area.
 RT UPPER LIMIT = +0.17 minutes of internal standard RT
 RT LOWER LIMIT = -0.17 minutes of internal standard RT

Column used to flag values outside QC limits with an asterisk.
 * Values outside of QC limits.

EPA 8260B

Form 2 & 8

Surrogate Recovery

Lab Name: APPL, Inc.

SDG No: 97923

Case No: 97923

Date Analyzed: 10/26/2021

Matrix: WATER

Instrument: Max

APPL ID.	Client Sample No.	SURROGATE: 1,2-DICHLOROETHANE-D4 (S)			SURROGATE: 4-BROMOFLUOROBENZENE (S)		
		Limits	Result	Qualifier	Limits	Result	Qualifier
211026BM-LCS	Lab Control Spike	81-118	104		85-114	104	
211026BM-LCSD	Lab Control SpikeD	81-118	101		85-114	102	
211026BM-BLK	Blank	81-118	99.7		85-114	99.8	
BA43836	ERH1835	81-118	100		85-114	96.9	
BA43837	ERH1836	81-118	97.2		85-114	96.1	

Comments: Batch: #86BTO-211026BM

Printed: 10/29/2021 4:54:19 AM
Form 2 & 8, Surrogate Recovery Summary

EPA 8260B

Form 2 & 8

Surrogate Recovery

Lab Name: APPL, Inc.
Case No: 97923
Matrix: WATER

SDG No: 97923
Date Analyzed: 10/26/2021
Instrument: Max

APPL ID.	Client Sample No.	SURROGATE: DIBROMOFLUOROMETHANE (S)			SURROGATE: TOLUENE-D8 (S)		
		Limits	Result	Qualifier	Limits	Result	Qualifier
211026BM-LCS	Lab Control Spike	80-119	103		89-112	102	
211026BM-LCSD	Lab Control SpikeD	80-119	103		89-112	101	
211026BM-BLK	Blank	80-119	99.8		89-112	98.9	
BA43836	ERH1835	80-119	104		89-112	100.0	
BA43837	ERH1836	80-119	101		89-112	102	

Comments: Batch: #86BTO-211026BM

Printed: 10/29/2021 4:54:19 AM
Form 2 & 8, Surrogate Recovery Summary

EPA 8260B

Form 4

Blank Summary

Lab Name: APPL, Inc.
Case No: 97923
Matrix: WATER
Blank ID: 211026BM-BLK

SDG No: 97923
Date Analyzed: 10/26/2021
Instrument: Max
Time Analyzed: 2320

APPL ID.	Client Sample No.	File ID.	Date Analyzed
211026BM-LCS	Lab Control Spike	1026M26	10/26/2021 2058
211026BM-LCSD	Lab Control Spiked	1026M27	10/26/2021 2126
211026BM-BLK	Blank	1026M31	10/26/2021 2320
BA43836	ERH1835	1026M35	10/27/2021 0113
BA43837	ERH1836	1026M36	10/27/2021 0141

Comments: Batch: #86BTO-211026BM

Printed: 10/29/2021 4:53:51 AM
Form 4, Blank Summary

Method Blank
EPA 8260B BTEX WATER

Blank Name/QCG: **211026W-43831 - 269592**
Batch ID: #86BTO-211026BM

APPL Inc.
908 North Temperance Avenue
Clovis, CA 93611

Sample Type	Analyte	Result	LOQ	LOD	DL	Units	Extraction Date	Analysis Date
BLANK	BENZENE	0.30 U	1.0	0.30	0.15	ug/L	10/26/2021	10/26/2021
BLANK	ETHYLBENZENE	0.50 U	1.0	0.50	0.23	ug/L	10/26/2021	10/26/2021
BLANK	TOLUENE	0.30 U	1.0	0.30	0.15	ug/L	10/26/2021	10/26/2021
BLANK	XYLENES (TOTAL)	0.30 U	2.0	0.30	0.15	ug/L	10/26/2021	10/26/2021
BLANK	SURROGATE: 1,2-DICHLOROET	99.7	81-118			%	10/26/2021	10/26/2021
BLANK	SURROGATE: 4-BROMOFLUORO	99.8	85-114			%	10/26/2021	10/26/2021
BLANK	SURROGATE: DIBROMOFLUOR	99.8	80-119			%	10/26/2021	10/26/2021
BLANK	SURROGATE: TOLUENE-D8 (S)	98.9	89-112			%	10/26/2021	10/26/2021

Quant Method:M1015W.M
Run #:1026M31
Instrument:Max
Sequence:211015
Initials: PAN

GC SC-Blank-REG MDLs-DOD
Printed: 10/29/2021 4:56:51 AM

EPA 8260B

Form 4

LCS Summary

Lab Name: APPL, Inc.

SDG No: 97923

Case No: 97923

Date Analyzed: 10/26/2021

Matrix: WATER

Instrument: Max

LCS ID: 211026BM-LCS

Time Analyzed: 2058

APPL ID.	Client Sample No.	File ID.	Date Analyzed
211026BM-LCS	Lab Control Spike	1026M26	10/26/2021 2058
211026BM-LCSD	Lab Control Spiked	1026M27	10/26/2021 2126
211026BM-BLK	Blank	1026M31	10/26/2021 2320
BA43836	ERH1835	1026M35	10/27/2021 0113
BA43837	ERH1836	1026M36	10/27/2021 0141

Comments: Batch: #86BTO-211026BM

Printed: 10/29/2021 4:52:49 AM
Form 4, LCS Summary

Laboratory Control Spike Recoveries

EPA 8260B BTEX WATER

APPL ID: 211026W-43831 LCS - 269592

Batch ID: #86BTO-211026BM

APPL Inc.

908 North Temperance Avenue

Clovis, CA 93611

Compound Name	Spike Lvl ug/L	SPK Result ug/L	DUP Result ug/L	SPK % Recovery	DUP % Recovery	Recovery Limits	RPD %	RPD Limits
BENZENE	10.00	10.4	9.29	104	92.9	79-120	11.3	20
ETHYLBENZENE	10.00	10.3	9.85	103	98.5	79-121	4.5	20
TOLUENE	10.00	10.3	9.63	103	96.3	80-121	6.7	20
XYLENES (TOTAL)	30.0	31.1	29.3	104	97.7	79-121	6.0	20

SURROGATE: 1,2-DICHLOROETHANE-D	25.0	26.0	25.2	104	101	81-118		
SURROGATE: 4-BROMOFLUOROBENZE	25.0	25.9	25.6	104	102	85-114		
SURROGATE: DIBROMOFLUOROMETH	25.0	25.7	25.8	103	103	80-119		
SURROGATE: TOLUENE-D8 (S)	25.0	25.4	25.2	102	101	89-112		

Comments: _____

<u>Primary</u>	<u>SPK</u>	<u>DUP</u>
Quant Method :	M1015W.M	M1015W.M
Extraction Date :	10/26/2021	10/26/2021
Analysis Date :	10/26/2021	10/26/2021
Instrument :	Max	Max
Run :	1026M26	1026M27
Initials :	PAN	

Form 5
Tune Summary

Lab Name: APPL Inc.
Case No: _____
Matrix: Water
ID: 1015M11.D

SDG No: _____
Date Analyzed: 10/15/2021
Instrument: Max
Time Analyzed: 14:44

Client Sample No.	APPL ID.	File ID.	Date Analyzed
1	0.3ug/L VOC STD 10/1	1015M12.D	10/15/2021 15:12
2	0.5ug/L VOC STD 10/1	1015M13.D	10/15/2021 15:41
3	1ug/L VOC STD 10/15/	1015M14.D	10/15/2021 16:09
4	2ug/L VOC STD 10/15/	1015M15.D	10/15/2021 16:38
5	5ug/L VOC STD 10/15/	1015M16.D	10/15/2021 17:06
6	10ug/L VOC STD 10/15	1015M17.D	10/15/2021 17:35
7	20ug/L VOC STD 10/15	1015M18.D	10/15/2021 18:03
8	40ug/L VOC STD 10/15	1015M19.D	10/15/2021 18:31
9	100ug/L VOC STD 10/1	1015M20.D	10/15/2021 19:00
10	(SS) 10ug/L VOC STD	1015M22.D	10/15/2021 19:57
11			
12			
13			
14			
15			
16			
17			
18			
19			
20			
21			
22			

m/e

50 15.0 - 40.0% of mass 95	<u>20.4</u>
75 30.0 - 60.0% of mas 95	<u>58.4</u>
95 Base peak, 100% relative abundance	<u>100.0</u>
96 5.0 - 9.0% of mass 95	<u>6.7</u>
173 Less than 2.0% of mass 174	<u>0.0</u>
174 50.0 - 200.0% of mass 95	<u>126.6</u>
175 5.0 - 9.0% of mass 174	<u>7.7</u>
176 95.0 - 101.0% of mass 174	<u>99.1</u>
177 5.0 - 9.0% of mass 176	<u>6.5</u>

8A
INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: APPL Inc. Contract: _____
 Lab Code: _____ SDG No.: _____
 Lab File ID (Standard): 1015M17.D Date Analyzed: 10/15/21
 Instrument ID: Max Time Analyzed: 17:35
 GC Column: _____ ID: _____ Heated Purge: (Y/N) _____

	Fluorobenzene (IS)		Chlorobenzene-D5 (IS)		1,4-Dichlorobenzene-D (IS)	
	AREA #	RT #	AREA #	RT #	AREA #	RT #
12 HOUR STD	377347	6.34	347072	9.50	236441	11.82
UPPER LIMIT	754694	6.51	694144	9.67	472882	11.99
LOWER LIMIT	188674	6.17	173536	9.33	118221	11.65
SAMPLE NO.						
01 0.3ug/L VOC STD 10/15/21	397342	6.34	352293	9.50	217437	11.82
02 0.5ug/L VOC STD 10/15/21	396824	6.34	348546	9.50	220294	11.82
03 1ug/L VOC STD 10/15/21	394605	6.34	355921	9.50	218264	11.82
04 2ug/L VOC STD 10/15/21	397741	6.34	352458	9.50	222724	11.82
05 5ug/L VOC STD 10/15/21	387411	6.34	344894	9.50	232454	11.82
06 10ug/L VOC STD 10/15/21	377347	6.34	347072	9.50	236441	11.82
07 20ug/L VOC STD 10/15/21	395871	6.34	351611	9.50	235162	11.82
08 40ug/L VOC STD 10/15/21	394795	6.34	356570	9.50	246902	11.82
09 100ug/L VOC STD 10/15/21	386789	6.34	357810	9.50	248989	11.82
10 (SS) 10ug/L VOC STD 10/15/21	407759	6.34	364241	9.50	235667	11.82
11						
12						
13						
14						
15						
16						
17						
18						
19						
20						
21						
22						

AREA UPPER LIMIT = +100% of internal standard area.
 AREA LOWER LIMIT = -50% of internal standard area.
 RT UPPER LIMIT = +0.17 minutes of internal standard RT
 RT LOWER LIMIT = -0.17 minutes of internal standard RT

Column used to flag values outside QC limits with an asterisk.
 * Values outside of QC limits.

Form 5
Tune Summary

Lab Name: APPL Inc.
Case No: 97923
Matrix: Water
ID: 1026M24.D

SDG No: 97923
Date Analyzed: 10/26/2021
Instrument: Max
Time Analyzed: 20:01

Client Sample No.	APPL ID.	File ID.	Date Analyzed	
1		211026B CCV 10ug/L	1026M25.D	10/26/2021 20:30
2	Lab Control Spike	211026B LCS 10ug/L	1026M26.D	10/26/2021 20:58
3	Lab Control SpikeD	211026B LCSD 10ug/L	1026M27.D	10/26/2021 21:26
4	Blank	211026B BLK	1026M31.D	10/26/2021 23:20
5	ERH1835	BA43836W01	1026M35.D	10/27/2021 1:13
6	ERH1836	BA43837W01	1026M36.D	10/27/2021 1:41
7		Ending CCV 10ug/L 10	1026M45.D	10/27/2021 5:55
8				
9				
10				
11				
12				
13				
14				
15				
16				
17				
18				
19				
20				
21				
22				

m/e

50 15.0 - 40.0% of mass 95	21.8
75 30.0 - 60.0% of mas 95	59.4
95 Base peak, 100% relative abundance	100.0
96 5.0 - 9.0% of mass 95	7.1
173 Less than 2.0% of mass 174	0.0
174 50.0 - 200.0% of mass 95	136.3
175 5.0 - 9.0% of mass 174	8.5
176 95.0 - 101.0% of mass 174	98.9
177 5.0 - 9.0% of mass 176	5.9

8A
INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: APPL Inc. Contract: _____
 Lab Code: _____ SDG No.: _____
 Lab File ID (Standard): 1026M25.D Date Analyzed: 10/26/21
 Instrument ID: Max Time Analyzed: 20:30
 GC Column: _____ ID: _____ Heated Purge: (Y/N) _____

		Fluorobenzene (IS)		Chlorobenzene-D5 (IS)		1,4-Dichlorobenzene-D (IS)	
		AREA #	RT #	AREA #	RT #	AREA #	RT #
12 HOUR STD		386002	6.37	343919	9.53	227821	11.85
UPPER LIMIT		772004	6.54	687838	9.70	455642	12.02
LOWER LIMIT		193001	6.20	171960	9.36	113911	11.68
SAMPLE NO.							
01	211026B CCV 10ug/L	386002	6.37	343919	9.53	227821	11.85
02	211026B LCS 10ug/L	384412	6.37	344538	9.53	230340	11.85
03	211026B LCSD 10ug/L	379540	6.37	341797	9.53	227568	11.85
04	211026B BLK	396235	6.37	350438	9.53	212898	11.85
05	BA43836W01	378804	6.37	343273	9.53	205124	11.85
06	BA43837W01	390312	6.37	341211	9.53	210844	11.84
07	Ending CCV 10ug/L 10/2	387172	6.37	351019	9.52	224090	11.84
08							
09							
10							
11							
12							
13							
14							
15							
16							
17							
18							
19							
20							
21							
22							

AREA UPPER LIMIT = +100% of internal standard area.
 AREA LOWER LIMIT = -50% of internal standard area.
 RT UPPER LIMIT = +0.17 minutes of internal standard RT
 RT LOWER LIMIT = -0.17 minutes of internal standard RT

Column used to flag values outside QC limits with an asterisk.
 * Values outside of QC limits.

EPA 8260B

Form 2 & 8

Surrogate Recovery

Lab Name: APPL, Inc.
Case No: 97923
Matrix: WATER

SDG No: 97923
Date Analyzed: 10/26/2021
Instrument: Max

APPL ID.	Client Sample No.	SURROGATE: 4-BROMOFLUOROBENZENE (S)			Limits	Result	Qualifier
		Limits	Result	Qualifier			
211026BM-LCS	Lab Control Spike	85-114	99.6				
211026BM-LCSD	Lab Control Spiked	85-114	100				
211026BM-BLK	Blank	85-114	99.8				
BA43836	ERH1835	85-114	98.3				
BA43837	ERH1836	85-114	97.5				

Comments: Batch: #GRO86-211026B

EPA 8260B

Form 4

Blank Summary

Lab Name: APPL, Inc.

SDG No: 97923

Case No: 97923

Date Analyzed: 10/26/2021

Matrix: WATER

Instrument: Max

Blank ID: 211026BM-BLK

Time Analyzed: 2320

APPL ID.	Client Sample No.	File ID.	Date Analyzed
211026BM-LCS	Lab Control Spike	1026M29	10/26/2021 2223
211026BM-LCSD	Lab Control Spiked	1026M30	10/26/2021 2251
211026BM-BLK	Blank	1026M31	10/26/2021 2320
BA43836	ERH1835	1026M35	10/27/2021 0113
BA43837	ERH1836	1026M36	10/27/2021 0141

Comments: Batch: #GRO86-211026B

Printed: 11/30/2021 1:35:15 PM
Form 4, Blank Summary

Method Blank
EPA 8260B GRO WATER

Blank Name/QCG: **211026W-43831 - 269634**
Batch ID: #GRO86-211026BM

APPL Inc.
908 North Temperance Avenue
Clovis, CA 93611

Sample Type	Analyte	Result	LOQ	LOD	DL	Units	Extraction Date	Analysis Date
BLANK	GASOLINE RANGE ORGANICS	18.0 U	20	18.0	8.6	ug/L	10/26/2021	10/26/2021
BLANK	SURROGATE: 4-BROMOFLUOR	99.8	85-114			%	10/26/2021	10/26/2021

Quant Method: SURR015W.
Run #: 1026M31
Instrument: Max
Sequence: 211015
Initials: DA

GC SC-Blank-REG MDLs-DOD
Printed: 11/30/2021 1:31:54 PM

EPA 8260B

Form 4

LCS Summary

Lab Name: APPL, Inc.
Case No: 97923
Matrix: WATER
LCS ID: 211026BM-LCS

SDG No: 97923
Date Analyzed: 10/26/2021
Instrument: Max
Time Analyzed: 2223

APPL ID.	Client Sample No.	File ID.	Date Analyzed
211026BM-LCS	Lab Control Spike	1026M29	10/26/2021 2223
211026BM-LCSD	Lab Control Spiked	1026M30	10/26/2021 2251
211026BM-BLK	Blank	1026M31	10/26/2021 2320
BA43836	ERH1835	1026M35	10/27/2021 0113
BA43837	ERH1836	1026M36	10/27/2021 0141

Comments: Batch: #GRO86-211026B

Laboratory Control Spike Recoveries

EPA 8260B GRO WATER

APPL ID: 211026W-43831 LCS - 269634
 Batch ID: #GRO86-211026BM

APPL Inc.
 908 North Temperance Avenue
 Clovis, CA 93611

Compound Name	Spike Lvl ug/L	SPK Result ug/L	DUP Result ug/L	SPK % Recovery	DUP % Recovery	Recovery Limits	RPD %	RPD Limits
GASOLINE RANGE ORGANICS	300	325	357	108	119	78-122	9.4	20
SURROGATE: 4-BROMOFLUOROBENZE	25.0	24.9	25.1	99.6	100	85-114		

Comments: _____

<u>Primary</u>	<u>SPK</u>	<u>DUP</u>
Quant Method :	SURR015W.M	SURR015W.M
Extraction Date :	10/26/2021	10/26/2021
Analysis Date :	10/26/2021	10/26/2021
Instrument :	Max	Max
Run :	1026M29	1026M30
Initials :	DA	

SW846 9060A

Form 4

Blank Summary

Lab Name: APPL, Inc.
Case No: 97923
Matrix: WATER
Blank ID: 211027A-BLK

SDG No: 97923
Date Analyzed: 10/27/2021
Instrument: TICTOC
Time Analyzed: 2210

APPL ID.	Client Sample No.	File ID.	Date Analyzed
211027A-BLK	Blank	15	10/27/2021 2210
211027A-LCS	Lab Control Spike	16	10/27/2021 2255
211027A-LCSD	Lab Control Spiked	17	10/27/2021 2341
BA43837	ERH1836	23	10/28/2021 0358

Comments: Batch: #TOCW5-211027A

WETLAB BLANK

APPL Inc.
908 North Temperance Avenue
Clovis, CA 93611

Method	Analyte	Result	LOQ	LOD	DL	Units	Prep Date	Analysis Date	QC Group
SW846 90	TOTAL ORGANIC C	0.350 U	0.93	0.350	0.130	mg/L	10/27/21	10/27/21	#TOCW5-211027A-BA43151

SW846 9060A

Form 4

LCS Summary

Lab Name: APPL, Inc.
Case No: 97923
Matrix: WATER
LCS ID: 211027A-LCS

SDG No: 97923
Date Analyzed: 10/27/2021
Instrument: TICTOC
Time Analyzed: 2255

APPL ID.	Client Sample No.	File ID.	Date Analyzed
211027A-BLK	Blank	15	10/27/2021 2210
211027A-LCS	Lab Control Spike	16	10/27/2021 2255
211027A-LCSD	Lab Control Spiked	17	10/27/2021 2341
BA43837	ERH1836	23	10/28/2021 0358

Comments: Batch: #TOCW5-211027A

Laboratory Control Spike Recoveries

WETLAB

APPL Inc.
 908 North Temperance Avenue
 Clovis, CA 93611

Method	Compound Name	Spike Lvl mg/L	SPK Res mg/L	DUP Res mg/L	SPK % Recov	DUP % Recov	RPD	RPD Max	QC Limits	Extract Date-Spk	Analysis Date-Spk	Extract Date-Dup	Analysis Date-Dup	QC Group
SW846 90	TOTAL ORGANIC CARBO	5.00	5.12	5.07	102	101	0.98	20	80-120	10/27/21	10/27/21	10/27/21	10/27/21	#TOCW5-211027A-BA431

Comments: _____

ORGANICS
Calibration Data

PAH by GCMS SIM
EPA 8270 SIM

Form 6
Initial Calibration

Lab Name: APPL, Inc.

SDG No:

Case No:

Initial Cal. Date: 10/19/2021

Matrix:

Instrument: KYLO

Initials: LS

1019K002.D 1019K003.D 1019K004.D 1019K005.D 1019K006.D 1019K007.D 1019K008.D 1019K009.D

	Compound	0.1	0.2	0.5	1	5	10	50	100			Avg	%RSD	Type	r^2	Q	MRF
1	I Naphthalene-D8(IS)																
2	TM Naphthalene	1.428	1.402	1.354	1.336	1.308	1.289	1.172	1.100			1.3	8.6	TM			0.700
3	S 2-Methylnaphthalene-D10 (2M)	1.359	1.337	1.324	1.305	1.316	1.159	1.222	1.192			1.3	5.9	S			
4	TM 2-Methylnaphthalene	0.7868	0.7804	0.7756	0.7764	0.7886	0.7810	0.7175	0.6825			0.76	5.1	TM			0.400
5	TM 1-Methylnaphthalene	0.8005	0.7905	0.7931	0.7961	0.7922	0.7806	0.7122	0.6797			0.77	6.0	TM			
6	I Acenaphthene-D10(IS)																
7	TM Acenaphthylene	5.288	5.373	5.323	5.258	5.439	5.405	4.863	4.456			5.2	6.6	TM			0.900
8	*TM Acenaphthene	1.497	1.444	1.402	1.372	1.398	1.381	1.266	1.207			1.4	6.8	*TM			0.900
9	TM Fluorene	1.615	1.645	1.600	1.590	1.642	1.640	1.521	1.456			1.6	4.2	TM			0.900
10	I Phenanthrene-D10(IS)																
11	TM Phenanthrene	1.510	1.398	1.383	1.377	1.403	1.374	1.309	1.253			1.4	5.4	TM			0.700
12	TM Anthracene	1.298	1.273	1.300	1.300	1.352	1.349	1.285	1.240			1.3	2.8	TM			0.700
13	S Fluoranthene-D10 (FRT)	2.023	1.976	1.895	1.904	2.032	1.918	1.953	1.890			1.9	2.9	S			
14	*TM Fluoranthene	2.169	2.135	2.136	2.147	2.255	2.226	2.086	1.944			2.1	4.4	*TM			0.600
15	I Chrysene-D12(IS)																
16	TM Pyrene	1.986	2.033	1.960	1.958	1.948	1.927	1.782	1.720			1.9	5.6	TM			0.600
17	TM Benz (a) anthracene	1.473	1.441	1.379	1.381	1.401	1.420	1.370	1.344			1.4	3.0	TM			0.800
18	TM Chrysene	1.754	1.672	1.608	1.574	1.554	1.516	1.410	1.375			1.6	8.1	TM			0.700
19	TML Indeno (1,2,3-cd) pyrene	1.687	1.326	1.360	1.404	1.015	1.052	1.169	1.168			1.3	17	TM	1.000		0.500
20	I Perylene-D12(IS)																
21	TM Benzo (b) fluoranthene	1.268	1.292	1.301	1.356	1.511	1.514	1.537	1.485			1.4	8.1	TM			0.700
22	TM Benzo (k) fluoranthene	1.593	1.558	1.636	1.632	1.670	1.730	1.578	1.484			1.6	4.6	TM			0.700
23	*TM Benzo (a) pyrene	1.254	1.223	1.224	1.265	1.442	1.484	1.454	1.383			1.3	8.3	*TM			0.700
24	TM Dibenz (a,h) anthracene	1.360	1.209	1.221	1.273	1.398	1.395	1.399	1.353			1.3	6.0	TM			0.400
25	TM Benzo (g,h,i) perylene	1.457	1.403	1.410	1.405	1.496	1.517	1.462	1.394			1.4	3.2	TM			0.500
26																	
27																	
28																	
29																	
30																	
31																	
32																	
33																	
34																	
35																	

Quantitation Report (Not Reviewed)

Data File : M:\KYLO\DATA\211019\1019K002.D
 Acq On : 19 Oct 21 14:09
 Sample : 0.1 ug/ml 10/13/21
 Misc :

Vial: 2
 Operator: LS
 Inst : KYLO
 Multiplr: 1.00

Quant Time: Oct 19 15:48 2021

Quant Results File: K1019.RES

Quant Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)
 Title : EPA 8270
 Last Update : Tue Oct 19 16:47:23 2021
 Response via : Initial Calibration
 DataAcq Meth : SIM_2

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Napthalene-D8 (IS)	3.92	136	10962	2.50000	ppb	0.00
6) Acenaphthene-D10 (IS)	5.86	164	5295	2.50000	ppb	0.00
10) Phenanthrene-D10 (IS)	7.56	188	8379	2.50000	ppb	0.00
15) Chrysene-D12 (IS)	10.63	240	9693	2.50000	ppb	0.01
20) Perylene-D12 (IS)	12.84	264	9009	2.50000	ppb	0.01
System Monitoring Compounds						
3) 2-Methylnaphthalene-D10 (2)	4.66	152	298	0.05323	ppb	0.00
Spiked Amount	5.000		Recovery	=	1.060%	
13) Fluoranthene-D10 (FRT)	8.94	212	339	0.05190	ppb	0.01
Spiked Amount	5.000		Recovery	=	1.040%	
Target Compounds						
2) Naphthalene	3.94	128	626	0.10994	ppb	99
4) 2-Methylnaphthalene	4.69	142	345	0.10338	ppb	100
5) 1-Methylnaphthalene	4.80	142	351	0.10422	ppb	99
7) Acenaphthylene	5.70	152	1120	0.10217	ppb	100
8) Acenaphthene	5.89	154	317	0.10918	ppb	99
9) Fluorene	6.49	166	342	0.10165	ppb	96
11) Phenanthrene	7.59	178	506	0.10973	ppb	100
12) Anthracene	7.65	178	435	0.09988	ppb	97
14) Fluoranthene	8.96	202	727	0.10149	ppb	98
16) Pyrene	9.22	202	770	0.10375	ppb	99
17) Benz (a) anthracene	10.62	228	571	0.10510	ppb	99
18) Chrysene	10.66	228	680	0.11258	ppb	96
19) Indeno (1,2,3-cd) pyrene	14.41	276	654	0.33399	ppb	# 88
22) Benzo (k) fluoranthene	12.21	252	574	-0.45104	ppb	97
23) Benzo (a) pyrene	12.75	252	452	-0.17190	ppb	95
24) Dibenz (a,h) anthracene	14.45	278	490	-0.04905	ppb	95
25) Benzo (g,h,i) perylene	14.71	276	525	-0.23039	ppb	98

Quantitation Report


Data File : M:\KYLO\DATA\211019\1019K002.D
Acq On : 19 Oct 21 14:09
Sample : 0.1 ug/ml 10/13/21
Misc :

Vial: 2
Operator: LS
Inst : KYLO
Multiplr: 1.00

Quant Time: Oct 19 15:48 2021

Quant Results File: K1019.RES

Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)
Title : EPA 8270
Last Update : Tue Nov 09 10:14:45 2021
Response via : Initial Calibration

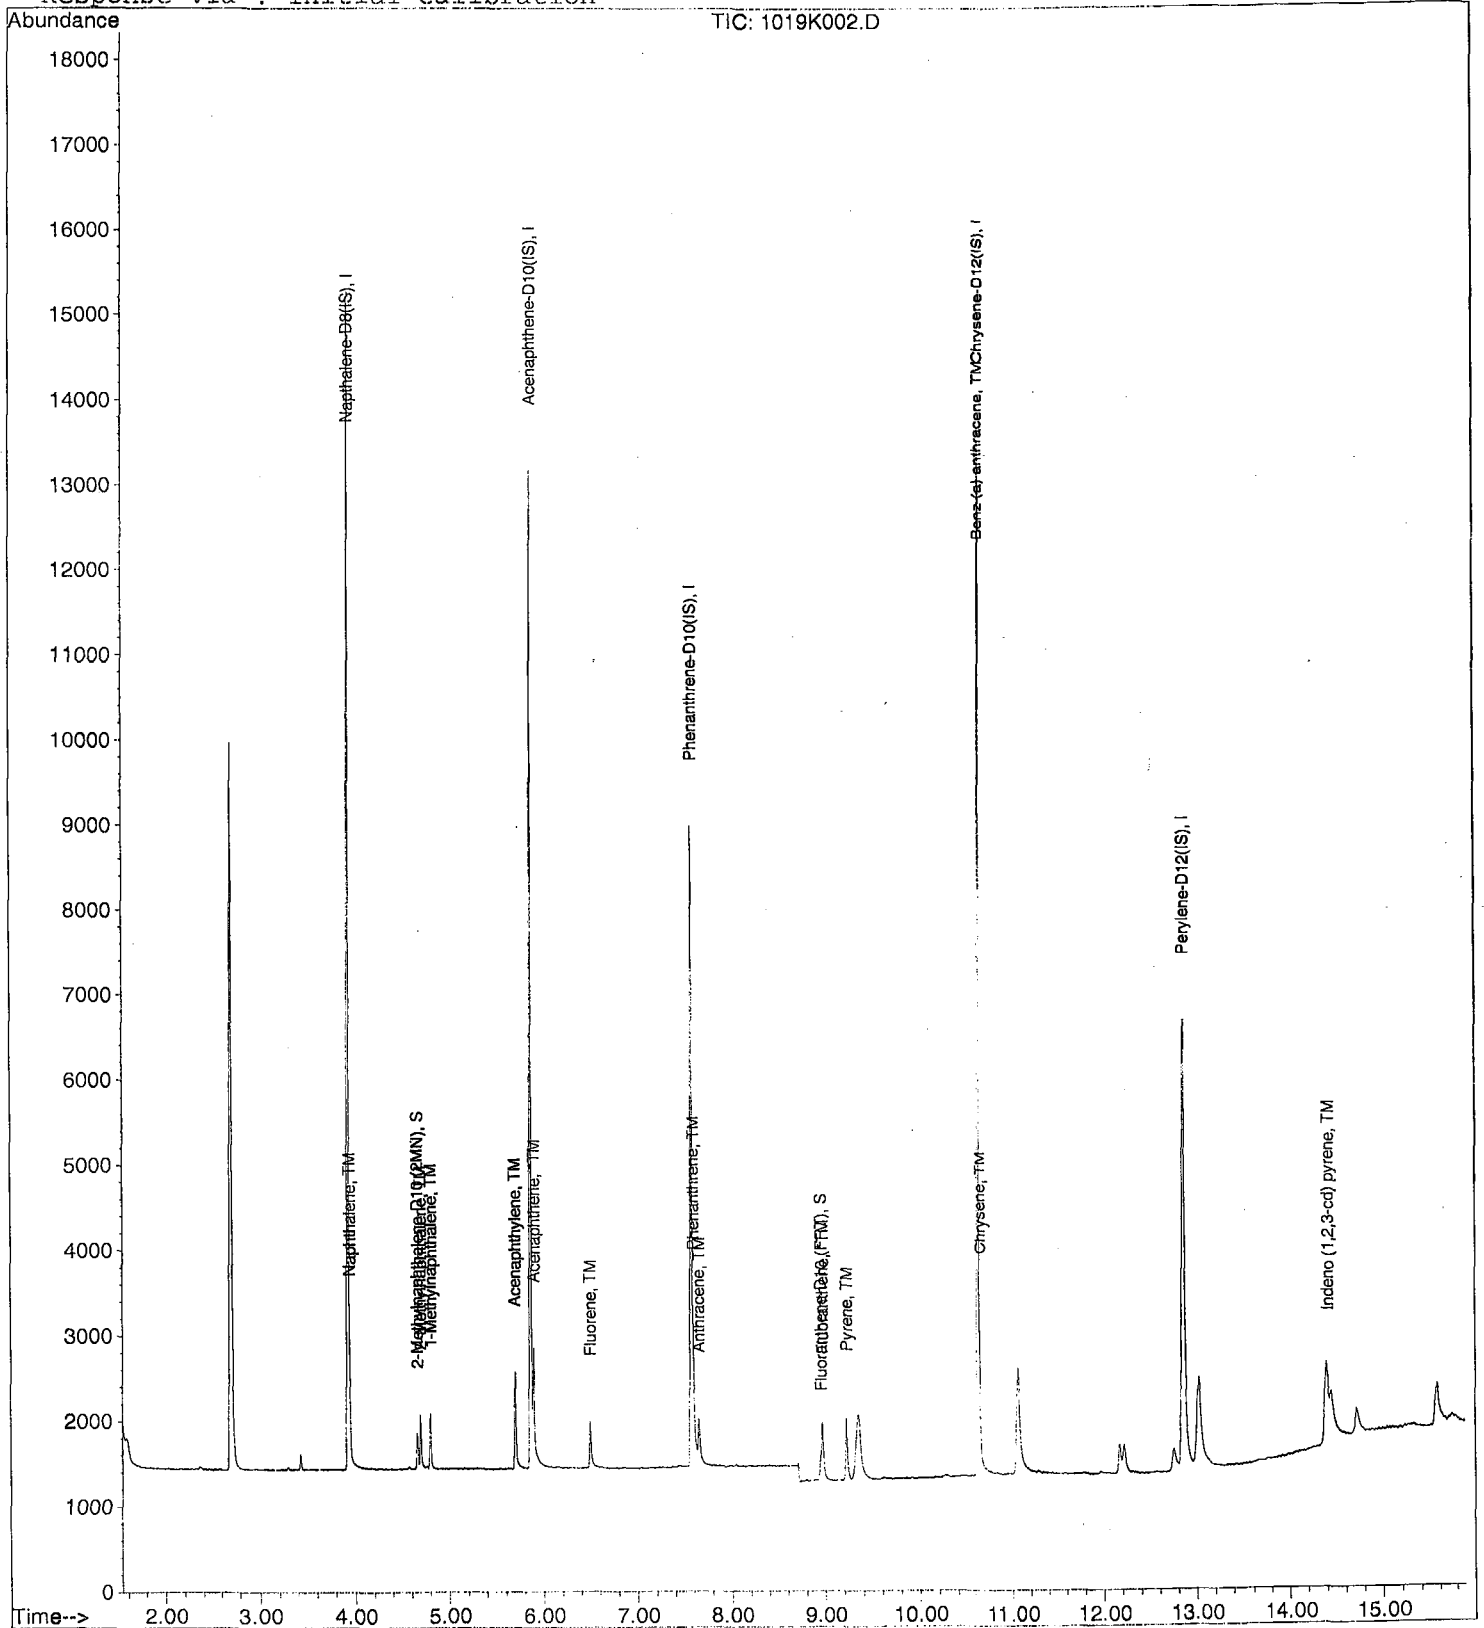

Data File : M:\KYLO\DATA\211019\1019K003.D
 Acq On : 19 Oct 21 14:29
 Sample : 0.2 ug/ml 10/13/21
 Misc :

Vial: 3
 Operator: LS
 Inst : KYLO
 Multiplr: 1.00

Quant Time: Oct 19 15:48 2021

Quant Results File: K1019.RES

Quant Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)
 Title : EPA 8270
 Last Update : Tue Oct 19 16:47:23 2021
 Response via : Initial Calibration
 DataAcq Meth : SIM_2

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Napthalene-D8 (IS)	3.92	136	11180	2.50000	ppb	0.00
6) Acenaphthenè-D10 (IS)	5.86	164	5495	2.50000	ppb	0.00
10) Phenanthrene-D10 (IS)	7.56	188	8995	2.50000	ppb	0.00
15) Chrysene-D12 (IS)	10.63	240	9881	2.50000	ppb	0.01
20) Perylene-D12 (IS)	12.84	264	8688	2.50000	ppb	0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 2-Methylnaphthalene-D10 (2)	4.66	152	598	0.10474	ppb	0.00
Spiked Amount	5.000		Recovery	=	2.100%	
13) Fluoranthene-D10 (FRT)	8.94	212	711	0.10140	ppb	0.01
Spiked Amount	5.000		Recovery	=	2.020%	

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Naphthalene	3.94	128	1254	0.21593	ppb	99
4) 2-Methylnaphthalene	4.69	142	698	0.20508	ppb	96
5) 1-Methylnaphthalene	4.80	142	707	0.20582	ppb	98
7) Acenaphthylene	5.69	152	2362	0.20763	ppb	100
8) Acenaphthene	5.89	154	635	0.21074	ppb	99
9) Fluorene	6.49	166	723	0.20706	ppb	100
11) Phenanthrene	7.59	178	1006	0.20323	ppb	100
12) Anthracene	7.65	178	916	0.19592	ppb	99
14) Fluoranthene	8.96	202	1536	0.19974	ppb	97
16) Pyrene	9.21	202	1607	0.21241	ppb	99
17) Benz (a) anthracene	10.62	228	1139	0.20566	ppb	98
18) Chrysene	10.66	228	1322	0.21470	ppb	99
19) Indeno (1,2,3-cd) pyrene	14.40	276	1048	0.41647	ppb	# 98
21) Benzo (b) fluoranthene	12.16	252	898	0.06057	ppb	98
22) Benzo (k) fluoranthene	12.21	252	1083	-0.34909	ppb	97
23) Benzo (a) pyrene	12.74	252	850	-0.08634	ppb	97
25) Benzo (g,h,i) perylene	14.71	276	975	-0.13423	ppb	96

Quantitation Report


Data File : M:\KYLO\DATA\211019\1019K003.D
Acq On : 19 Oct 21 14:29
Sample : 0.2 ug/ml 10/13/21
Misc :

Vial: 3
Operator: LS
Inst : KYLO
Multiplr: 1.00

Quant Time: Oct 19 15:48 2021

Quant Results File: K1019.RES

Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)
Title : EPA 8270
Last Update : Tue Nov 09 10:14:45 2021
Response via : Initial Calibration

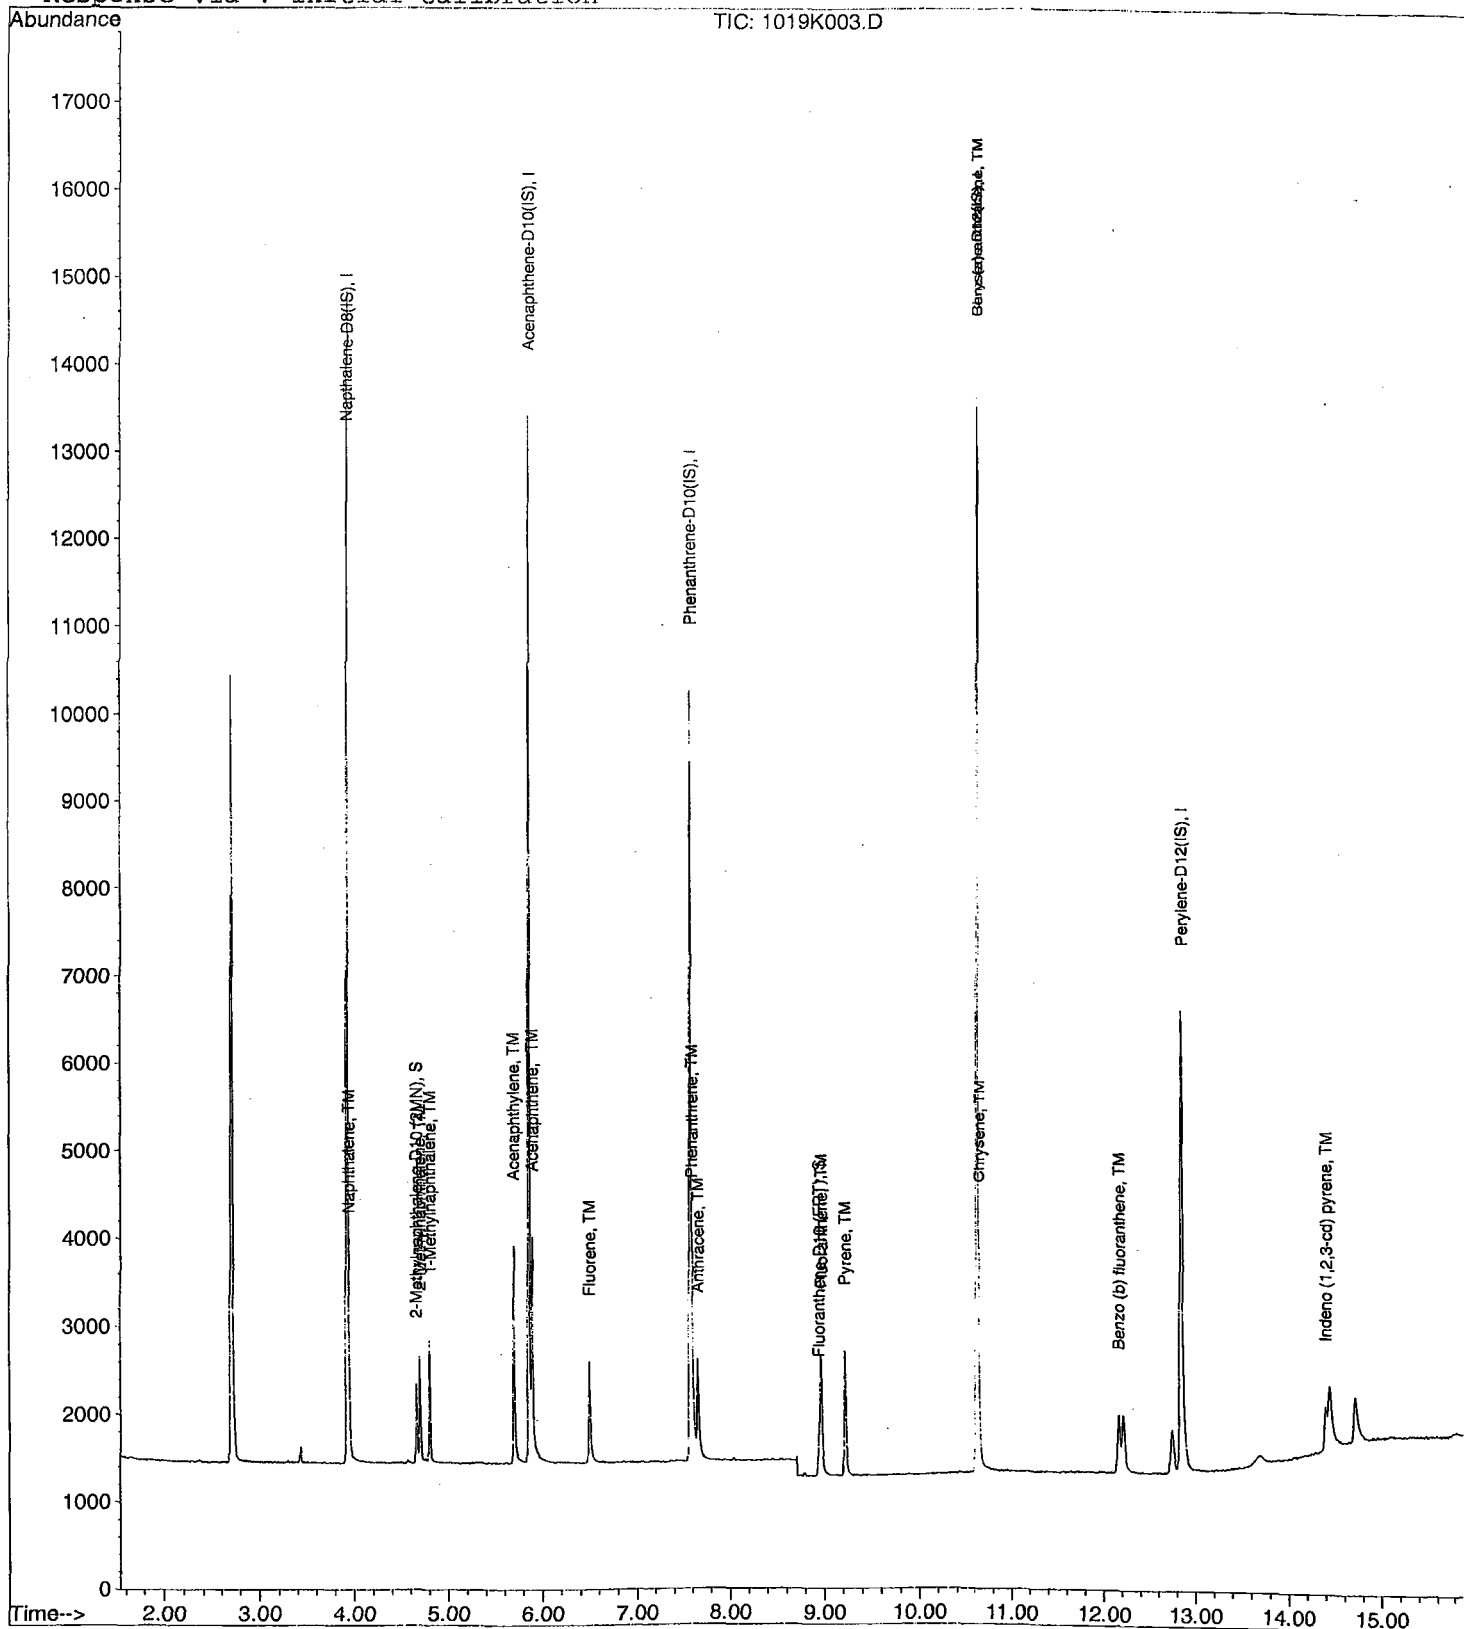

Quantitation Report (Not Reviewed)

Data File : M:\KYLO\DATA\211019\1019K004.D
 Acq On : 19 Oct 21 14:49
 Sample : 0.5 ug/ml 10/13/21
 Misc :

Vial: 4
 Operator: LS
 Inst : KYLO
 Multiplr: 1.00

Quant Time: Oct 19 15:48 2021

Quant Results File: K1019.RES

Quant Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)
 Title : EPA 8270
 Last Update : Tue Oct 19 16:47:23 2021
 Response via : Initial Calibration
 DataAcq Meth : SIM_2

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Napthalene-D8 (IS)	3.92	136	11385	2.50000	ppb	0.00
6) Acenaphthene-D10 (IS)	5.86	164	5536	2.50000	ppb	0.00
10) Phenanthrene-D10 (IS)	7.56	188	8686	2.50000	ppb	0.00
15) Chrysene-D12 (IS)	10.62	240	9708	2.50000	ppb	0.00
20) Perylene-D12 (IS)	12.84	264	8669	2.50000	ppb	0.00

System Monitoring Compounds

3) 2-Methylnaphthalene-D10 (2)	4.66	152	1507	0.25921	ppb	0.00
Spiked Amount	5.000		Recovery	=	5.180%	
13) Fluoranthene-D10 (FRT)	8.94	212	1646	0.24309	ppb	0.00
Spiked Amount	5.000		Recovery	=	4.860%	

Target Compounds

	R.T.	QIon	Response	Conc	Units	Qvalue
2) Naphthalene	3.94	128	3083	0.52131	ppb	99
4) 2-Methylnaphthalene	4.69	142	1766	0.50952	ppb	99
5) 1-Methylnaphthalene	4.80	142	1806	0.51630	ppb	96
7) Acenaphthylene	5.69	152	5894	0.51427	ppb	100
8) Acenaphthene	5.89	154	1552	0.51126	ppb	100
9) Fluorene	6.49	166	1772	0.50373	ppb	99
11) Phenanthrene	7.59	178	2402	0.50250	ppb	99
12) Anthracene	7.65	178	2259	0.50035	ppb	99
14) Fluoranthene	8.96	202	3711	0.49974	ppb	99
16) Pyrene	9.21	202	3805	0.51191	ppb	98
17) Benz (a) anthracene	10.61	228	2678	0.49216	ppb	99
18) Chrysene	10.65	228	3122	0.51607	ppb	99
19) Indeno (1,2,3-cd) pyrene	14.39	276	2640	0.77101	ppb	# 97
21) Benzo (b) fluoranthene	12.15	252	2255	0.32301	ppb	100
23) Benzo (a) pyrene	12.74	252	2122	0.17741	ppb	99
24) Dibenz (a,h) anthracene	14.43	278	2117	0.29983	ppb	99
25) Benzo (g,h,i) perylene	14.70	276	2445	0.16843	ppb	100

Quantitation Report


Data File : M:\KYLO\DATA\211019\1019K004.D
Acq On : 19 Oct 21 14:49
Sample : 0.5 ug/ml 10/13/21
Misc :

Vial: 4
Operator: LS
Inst : KYLO
Multiplr: 1.00

Quant Time: Oct 19 15:48 2021

Quant Results File: K1019.RES

Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)
Title : EPA 8270
Last Update : Tue Nov 09 10:14:45 2021
Response via : Initial Calibration

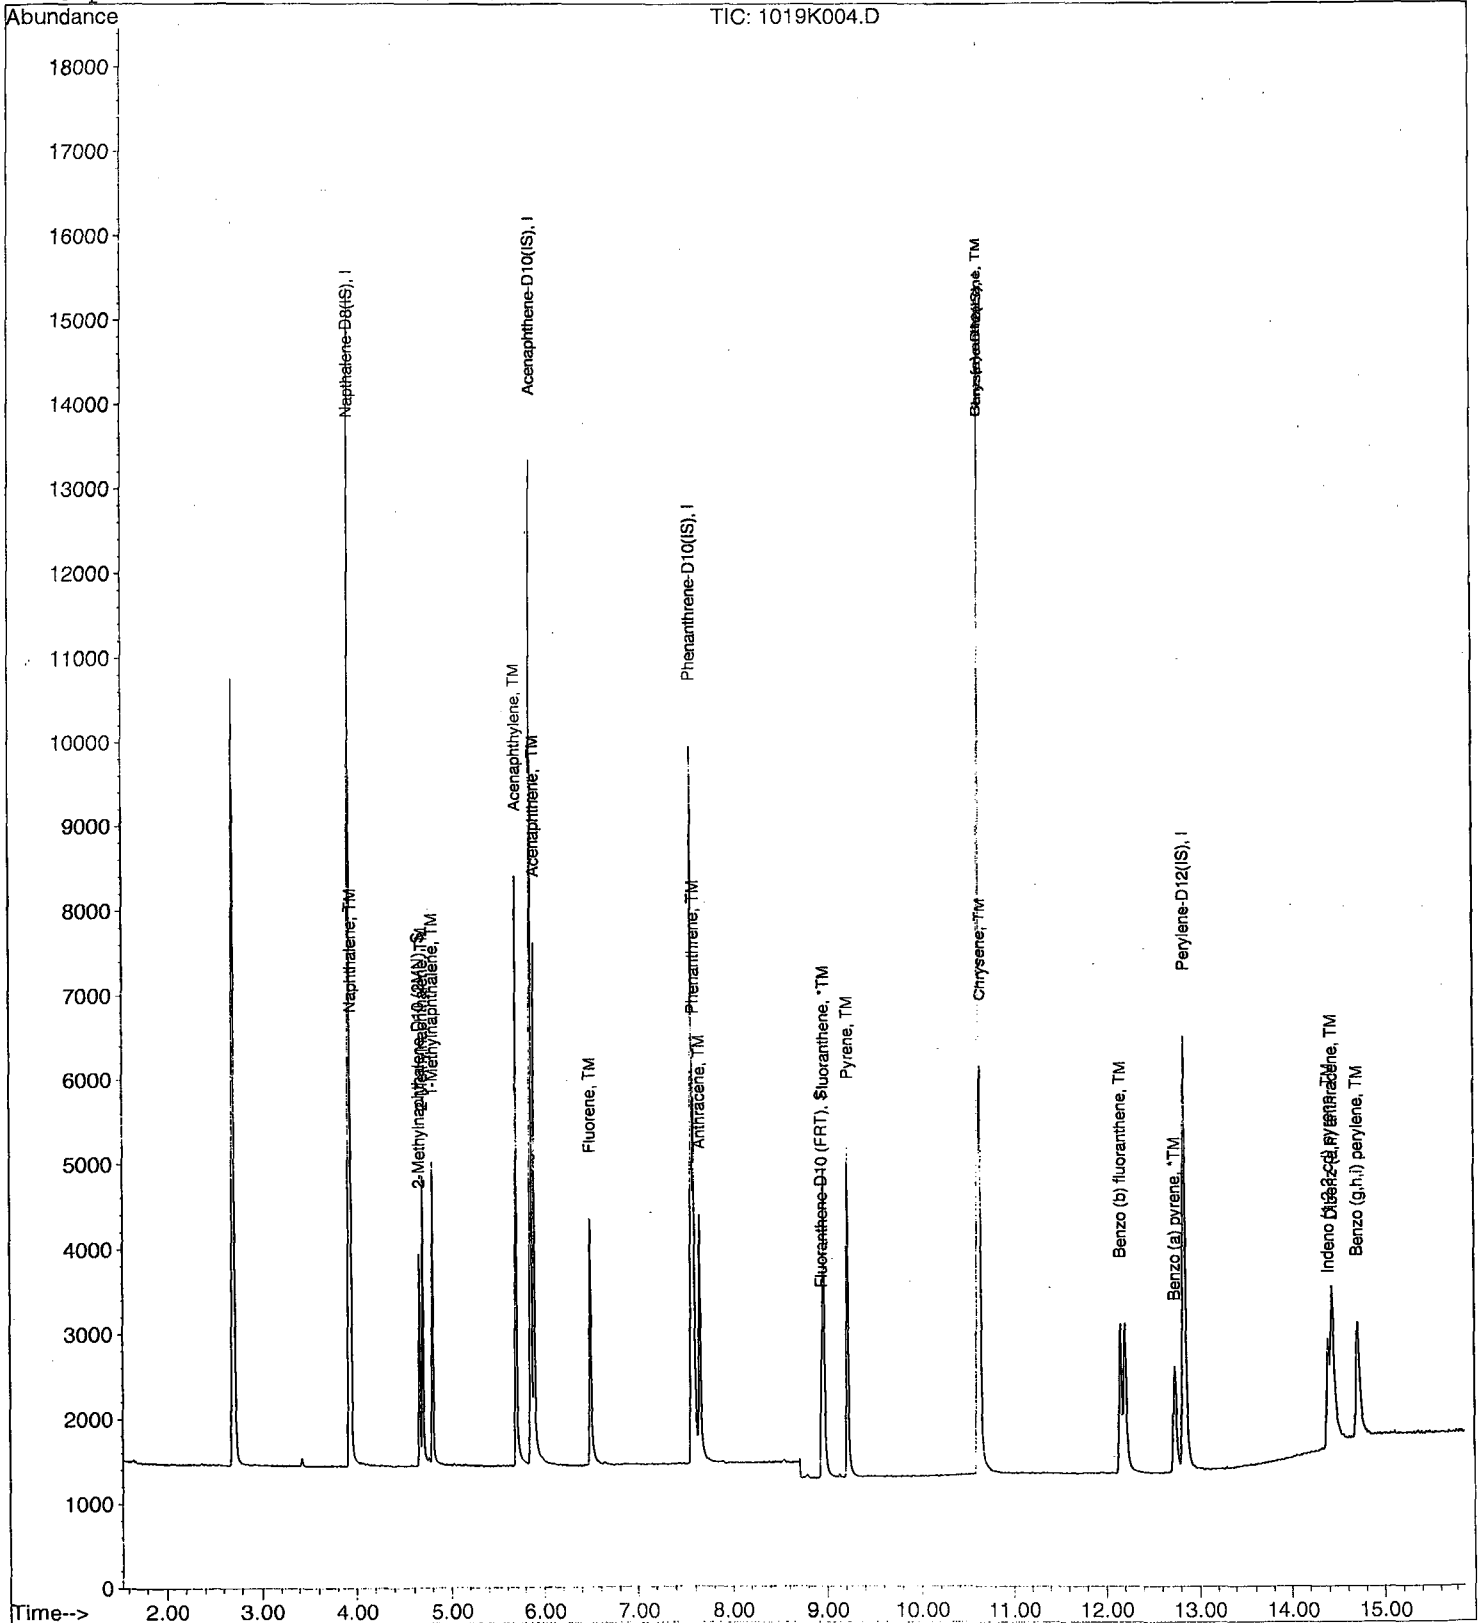

Quantitation Report (Not Reviewed)

Data File : M:\KYLO\DATA\211019\1019K005.D
 Acq On : 19 Oct 21 15:09
 Sample : 1 ug/ml 10/13/21
 Misc :

Vial: 5
 Operator: LS
 Inst : KYLO
 Multiplr: 1.00

Quant Time: Oct 19 15:48 2021

Quant Results File: K1019.RES

Quant Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)
 Title : EPA 8270
 Last Update : Tue Oct 19 16:47:23 2021
 Response via : Initial Calibration
 DataAcq Meth : SIM_2

Internal Standards	R.T.	QI on	Response	Conc	Units	Dev(Min)
1) Naphthalene-D8 (IS)	3.92	136	11032	2.50000	ppb	0.00
6) Acenaphthene-D10 (IS)	5.86	164	5365	2.50000	ppb	0.00
10) Phenanthrene-D10 (IS)	7.56	188	8424	2.50000	ppb	0.00
15) Chrysene-D12 (IS)	10.63	240	9455	2.50000	ppb	0.01
20) Perylene-D12 (IS)	12.84	264	8423	2.50000	ppb	0.01

System Monitoring Compounds

3) 2-Methylnaphthalene-D10 (2)	4.66	152	2880	0.51122	ppb	0.00
Spiked Amount	5.000		Recovery	=	10.220%	
13) Fluoranthene-D10 (FRT)	8.94	212	3208	0.48851	ppb	0.00
Spiked Amount	5.000		Recovery	=	9.780%	

Target Compounds

	R.T.	QI on	Response	Conc	Units	Qvalue
2) Naphthalene	3.94	128	5894	1.02851	ppb	99
4) 2-Methylnaphthalene	4.69	142	3426	1.02008	ppb	99
5) 1-Methylnaphthalene	4.80	142	3513	1.03643	ppb	98
7) Acenaphthylene	5.70	152	11284	1.01594	ppb	99
8) Acenaphthene	5.89	154	2945	1.00106	ppb	97
9) Fluorene	6.49	166	3412	1.00086	ppb	99
11) Phenanthrene	7.59	178	4641	1.00109	ppb	99
12) Anthracene	7.65	178	4379	1.00008	ppb	100
14) Fluoranthene	8.96	202	7234	1.00447	ppb	100
16) Pyrene	9.21	202	7407	1.02317	ppb	99
17) Benz (a) anthracene	10.61	228	5224	0.98576	ppb	99
18) Chrysene	10.65	228	5954	1.01055	ppb	99
19) Indeno (1,2,3-cd) pyrene	14.39	276	5309	1.38990	ppb	# 90
21) Benzo (b) fluoranthene	12.15	252	4568	0.79546	ppb	99
22) Benzo (k) fluoranthene	12.21	252	5497	0.53419	ppb	98
23) Benzo (a) pyrene	12.74	252	4263	0.64650	ppb	99
24) Dibenz (a,h) anthracene	14.44	278	4288	0.78667	ppb	99
25) Benzo (g,h,i) perylene	14.71	276	4733	0.66726	ppb	99

Quantitation Report


Data File : M:\KYLO\DATA\211019\1019K005.D
Acq On : 19 Oct 21 15:09
Sample : 1 ug/ml 10/13/21
Misc :

Vial: 5
Operator: LS
Inst : KYLO
Multiplr: 1.00

Quant Time: Oct 19 15:48 2021

Quant Results File: K1019.RES

Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)
Title : EPA 8270
Last Update : Tue Nov 09 10:14:45 2021
Response via : Initial Calibration

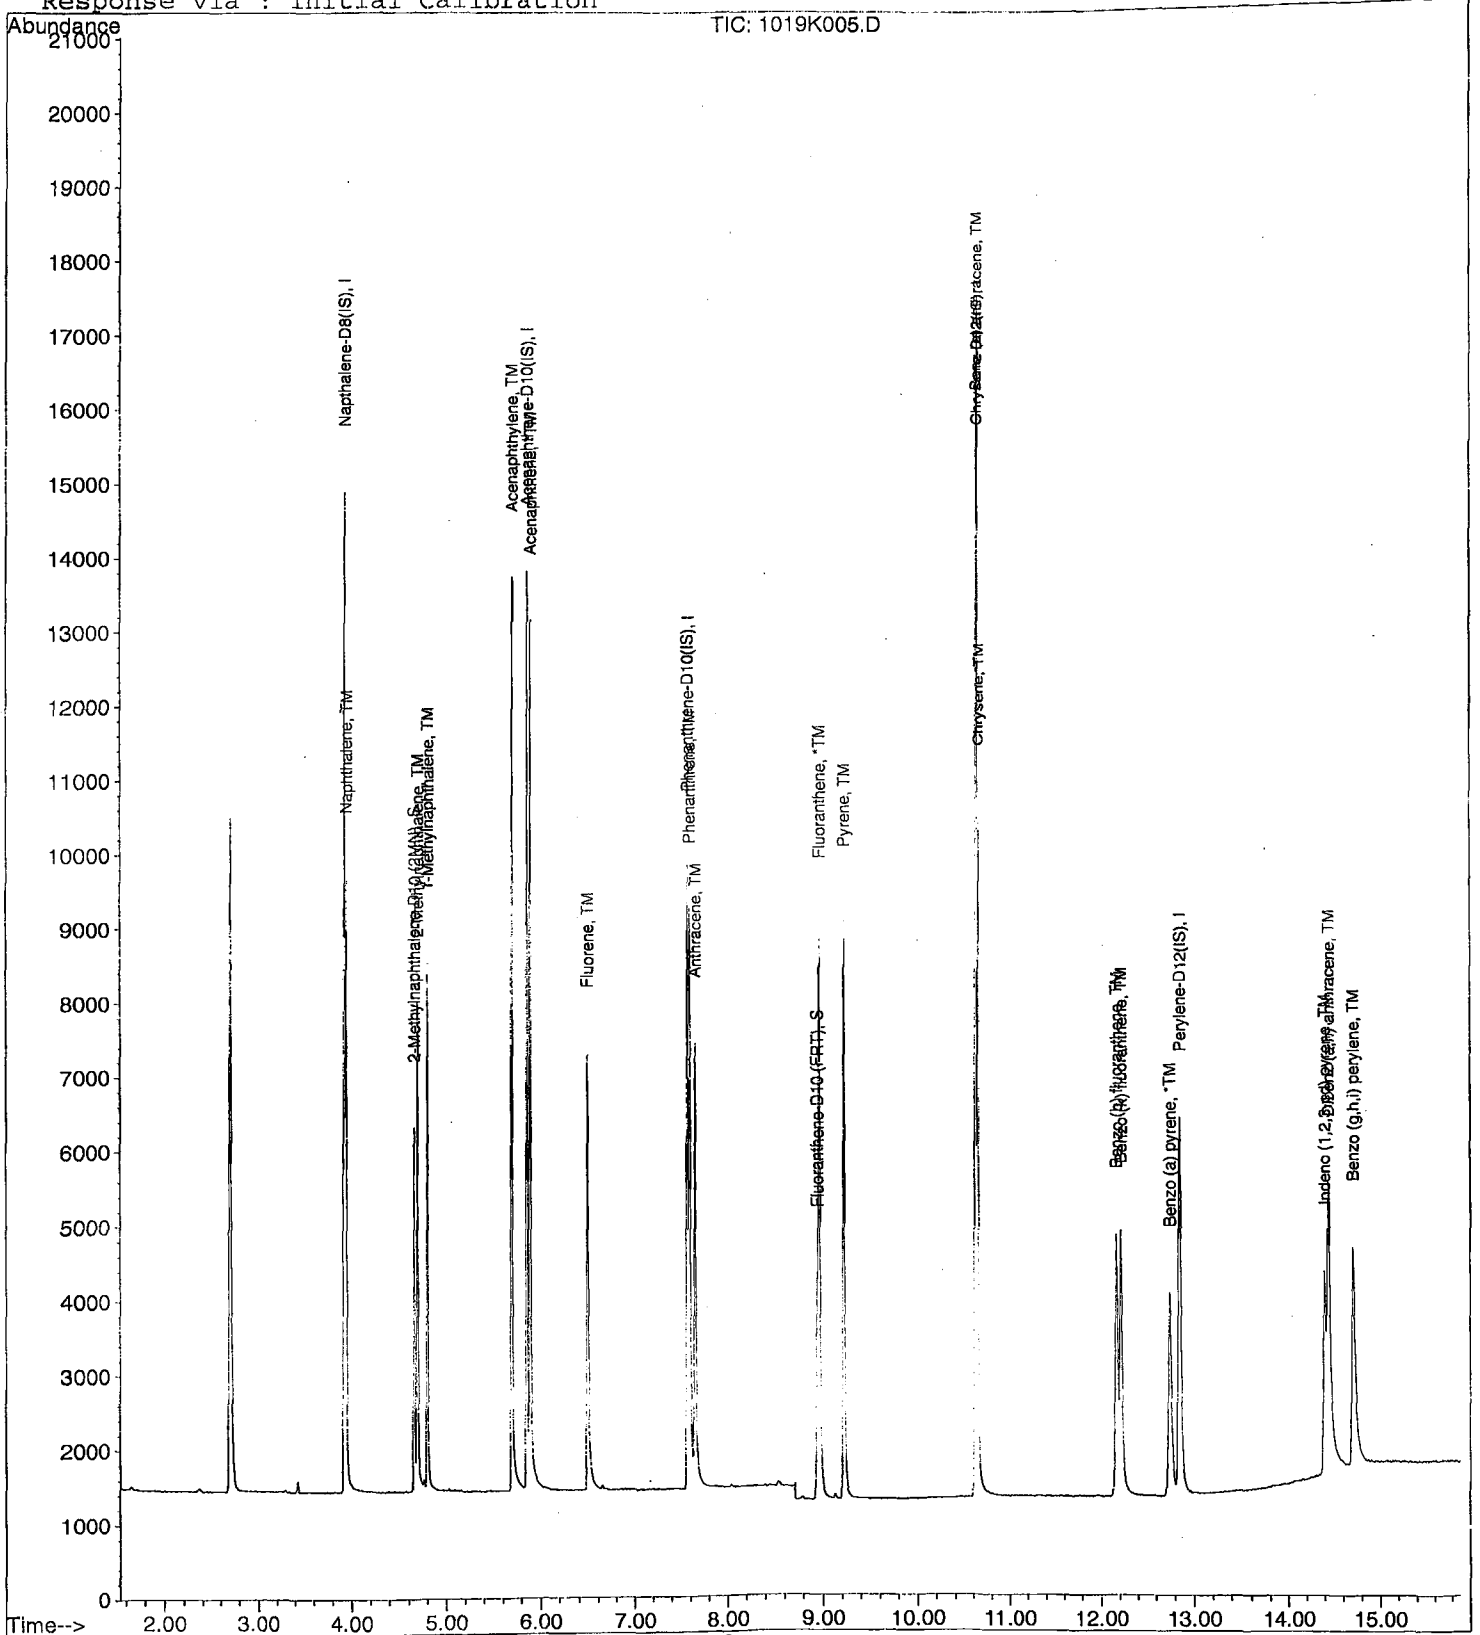

Quantitation Report (Not Reviewed)

Data File : M:\KYLO\DATA\211019\1019K006.D
 Acq On : 19 Oct 21 15:29
 Sample : 5 ug/ml 10/13/21
 Misc :

Vial: 6
 Operator: LS
 Inst : KYLO
 Multiplr: 1.00

Quant Time: Oct 19 15:48 2021

Quant Results File: K1019.RES

Quant Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)
 Title : EPA 8270
 Last Update : Tue Oct 19 16:47:23 2021
 Response via : Initial Calibration
 DataAcq Meth : SIM_2

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Naphthalene-D8 (IS)	3.92	136	11022	2.50000	ppb	0.00
6) Acenaphthene-D10 (IS)	5.86	164	5414	2.50000	ppb	0.00
10) Phenanthrene-D10 (IS)	7.56	188	8482	2.50000	ppb	0.00
15) Chrysene-D12 (IS)	10.62	240	10015	2.50000	ppb	0.00
20) Perylene-D12 (IS)	12.83	264	8704	2.50000	ppb	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 2-Methylnaphthalene-D10 (2)	4.66	152	14500	2.57619	ppb	0.00
Spiked Amount 5.000			Recovery =	51.520%		
13) Fluoranthene-D10 (FRT)	8.93	212	17235	2.60659	ppb	0.00
Spiked Amount 5.000			Recovery =	52.140%		

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Naphthalene	3.94	128	28832	5.03578	ppb	100
4) 2-Methylnaphthalene	4.69	142	17384	5.18072	ppb	100
5) 1-Methylnaphthalene	4.80	142	17464	5.15700	ppb	100
7) Acenaphthylene	5.69	152	58890	5.25410	ppb	100
8) Acenaphthene	5.89	154	15136	5.09845	ppb	100
9) Fluorene	6.49	166	17780	5.16829	ppb	100
11) Phenanthrene	7.59	178	23796	5.09785	ppb	100
12) Anthracene	7.64	178	22931	5.20117	ppb	100
14) Fluoranthene	8.95	202	38260	5.27621	ppb	100
16) Pyrene	9.21	202	39012	5.08763	ppb	100
17) Benz (a) anthracene	10.61	228	28070	5.00058	ppb	100
18) Chrysene	10.65	228	31118	4.98620	ppb	100
19) Indeno (1,2,3-cd) pyrene	14.38	276	20323	4.52699	ppb	100
21) Benzo (b) fluoranthene	12.14	252	26309	4.94784	ppb	100
22) Benzo (k) fluoranthene	12.19	252	29066	5.02910	ppb	100
23) Benzo (a) pyrene	12.73	252	25103	4.91484	ppb	100
24) Dibenz (a,h) anthracene	14.42	278	24331	4.98885	ppb	100
25) Benzo (g,h,i) perylene	14.69	276	26049	4.99985	ppb	100

Quantitation Report


Data File : M:\KYLO\DATA\211019\1019K006.D
Acq On : 19 Oct 21 15:29
Sample : 5 ug/ml 10/13/21
Misc :

Vial: 6
Operator: LS
Inst : KYLO
Multiplr: 1.00

Quant Time: Oct 19 15:48 2021

Quant Results File: K1019.RES

Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)
Title : EPA 8270
Last Update : Tue Nov 09 10:14:45 2021
Response via : Initial Calibration

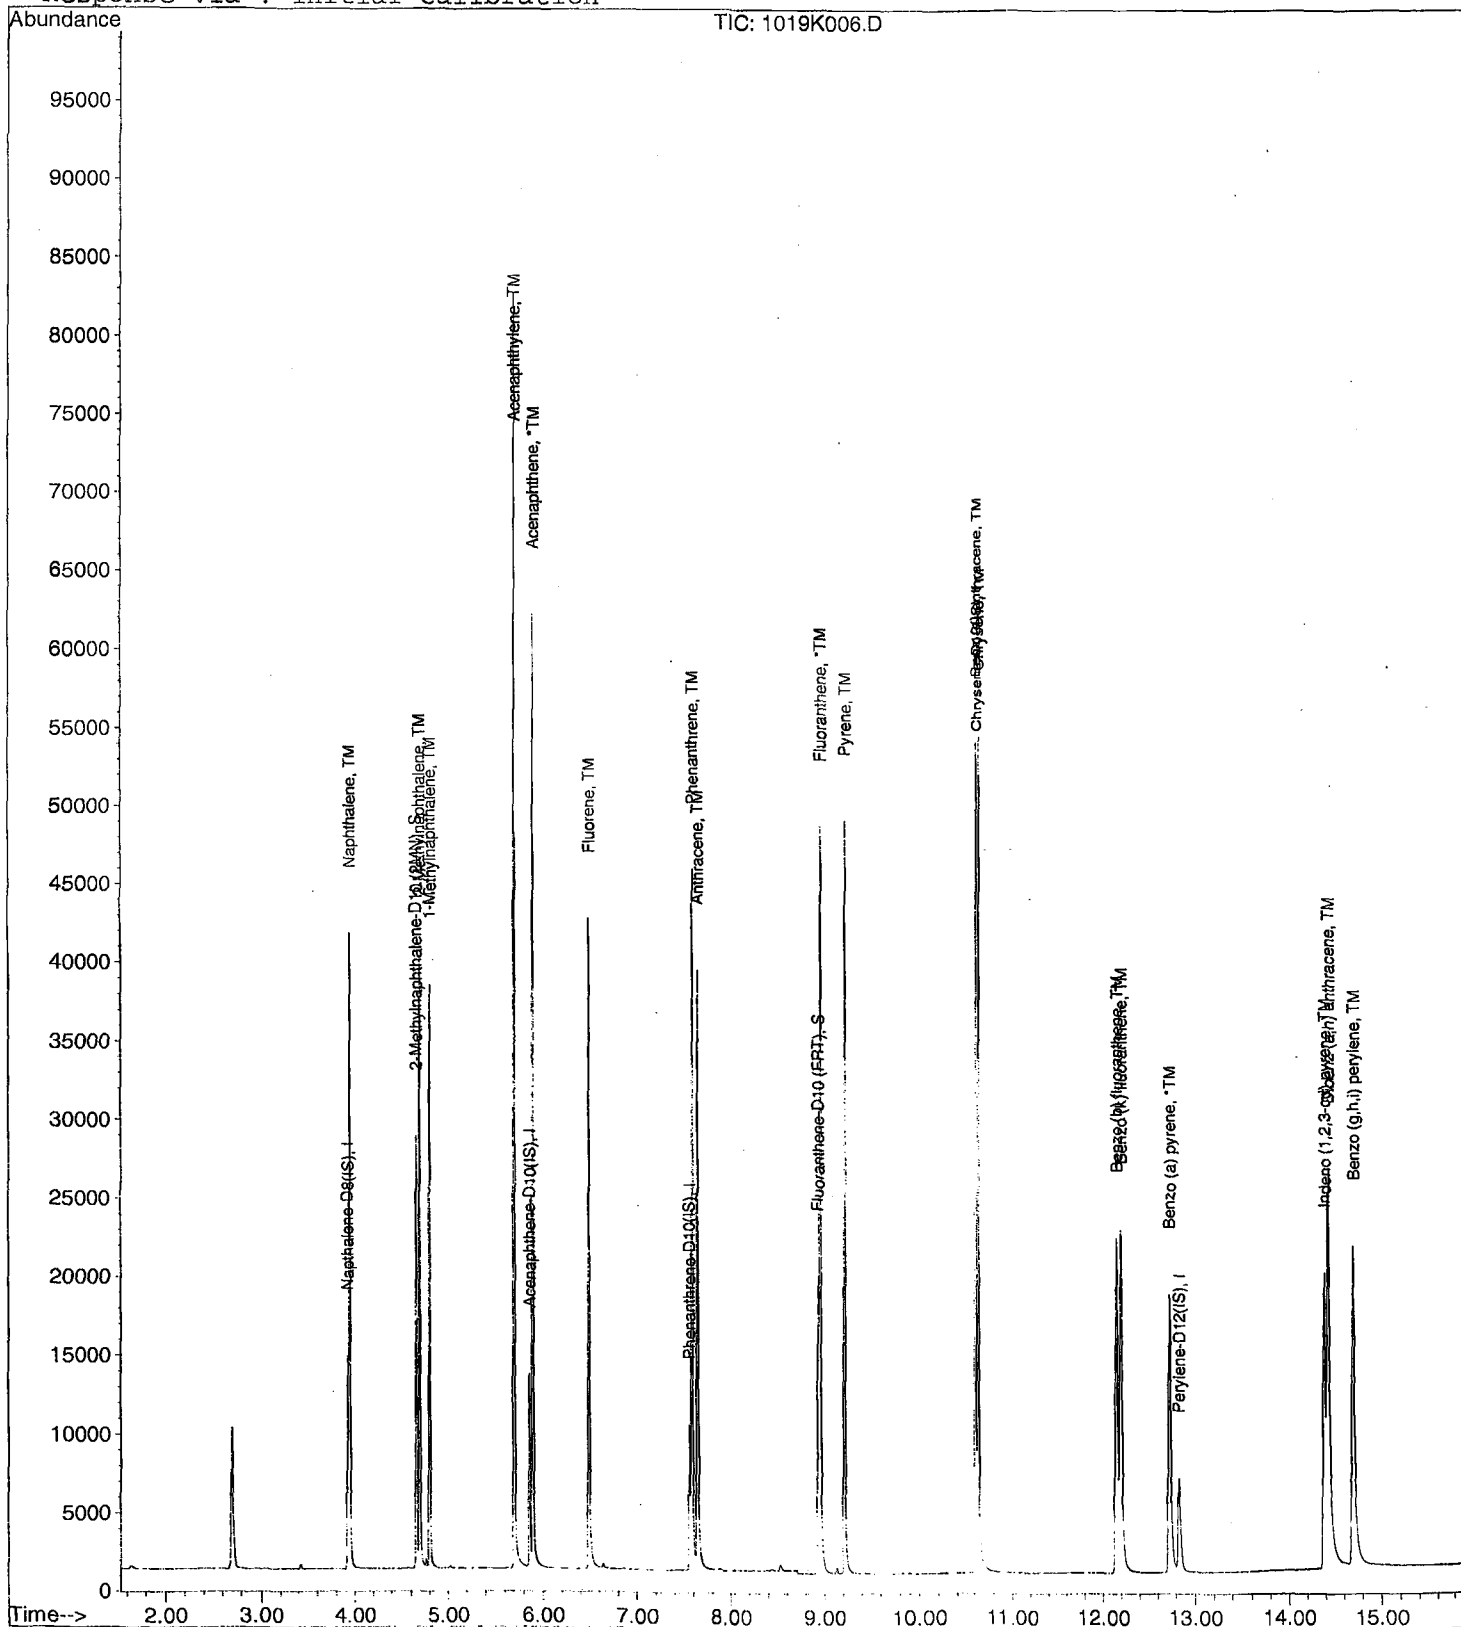

Quantitation Report (Not Reviewed)

Data File : M:\KYLO\DATA\211019\1019K007.D
 Acq On : 19 Oct 21 15:49
 Sample : 10 ug/ml 10/13/21
 Misc :

Vial: 7
 Operator: LS
 Inst : KYLO
 Multiplr: 1.00

Quant Time: Oct 19 15:49 2021

Quant Results File: K1019.RES

Quant Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)
 Title : EPA 8270
 Last Update : Tue Oct 19 16:47:23 2021
 Response via : Initial Calibration
 DataAcq Meth : SIM_2

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Napthalene-D8 (IS)	3.92	136	11510	2.50000	ppb	0.00
6) Acenaphthene-D10 (IS)	5.86	164	5675	2.50000	ppb	0.00
10) Phenanthrene-D10 (IS)	7.56	188	8972	2.50000	ppb	0.00
15) Chrysene-D12 (IS)	10.62	240	10664	2.50000	ppb	0.00
20) Perylene-D12 (IS)	12.83	264	9232	2.50000	ppb	0.00
System Monitoring Compounds						
3) 2-Methylnaphthalene-D10 (2)	4.66	152	26676	4.53854	ppb	0.00
Spiked Amount	5.000		Recovery	=	90.780%	
13) Fluoranthene-D10 (FRT)	8.93	212	34413	4.92032	ppb	0.00
Spiked Amount	5.000		Recovery	=	98.400%	
Target Compounds						
2) Naphthalene	3.94	128	59354	9.92720	ppb	100
4) 2-Methylnaphthalene	4.69	142	35959	10.26203	ppb	100
5) 1-Methylnaphthalene	4.80	142	35938	10.16232	ppb	100
7) Acenaphthylene	5.69	152	122704	10.44402	ppb	100
8) Acenaphthene	5.89	154	31359	10.07724	ppb	99
9) Fluorene	6.49	166	37236	10.32596	ppb	99
11) Phenanthrene	7.59	178	49310	9.98682	ppb	100
12) Anthracene	7.64	178	48395	10.37738	ppb	100
14) Fluoranthene	8.95	202	79898	10.41651	ppb	100
16) Pyrene	9.21	202	82191	10.06635	ppb	100
17) Benz (a) anthracene	10.61	228	60563	10.13248	ppb	100
18) Chrysene	10.65	228	64649	9.72861	ppb	99
19) Indeno (1,2,3-cd) pyrene	14.38	276	44868	9.18248	ppb	# 99
21) Benzo (b) fluoranthene	12.14	252	55900	10.02449	ppb	99
22) Benzo (k) fluoranthene	12.19	252	63873	11.01716	ppb	99
23) Benzo (a) pyrene	12.73	252	54783	10.38939	ppb	99
24) Dibenz (a,h) anthracene	14.42	278	51533	10.11061	ppb	98
25) Benzo (g,h,i) perylene	14.69	276	56013	10.47964	ppb	98

Quantitation Report


Data File : M:\KYLO\DATA\211019\1019K007.D
Acq On : 19 Oct 21 15:49
Sample : 10 ug/ml 10/13/21
Misc :

Vial: 7
Operator: LS
Inst : KYLO
Multiplr: 1.00

Quant Time: Oct 19 15:49 2021

Quant Results File: K1019.RES

Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)
Title : EPA 8270
Last Update : Tue Nov 09 10:14:45 2021
Response via : Initial Calibration

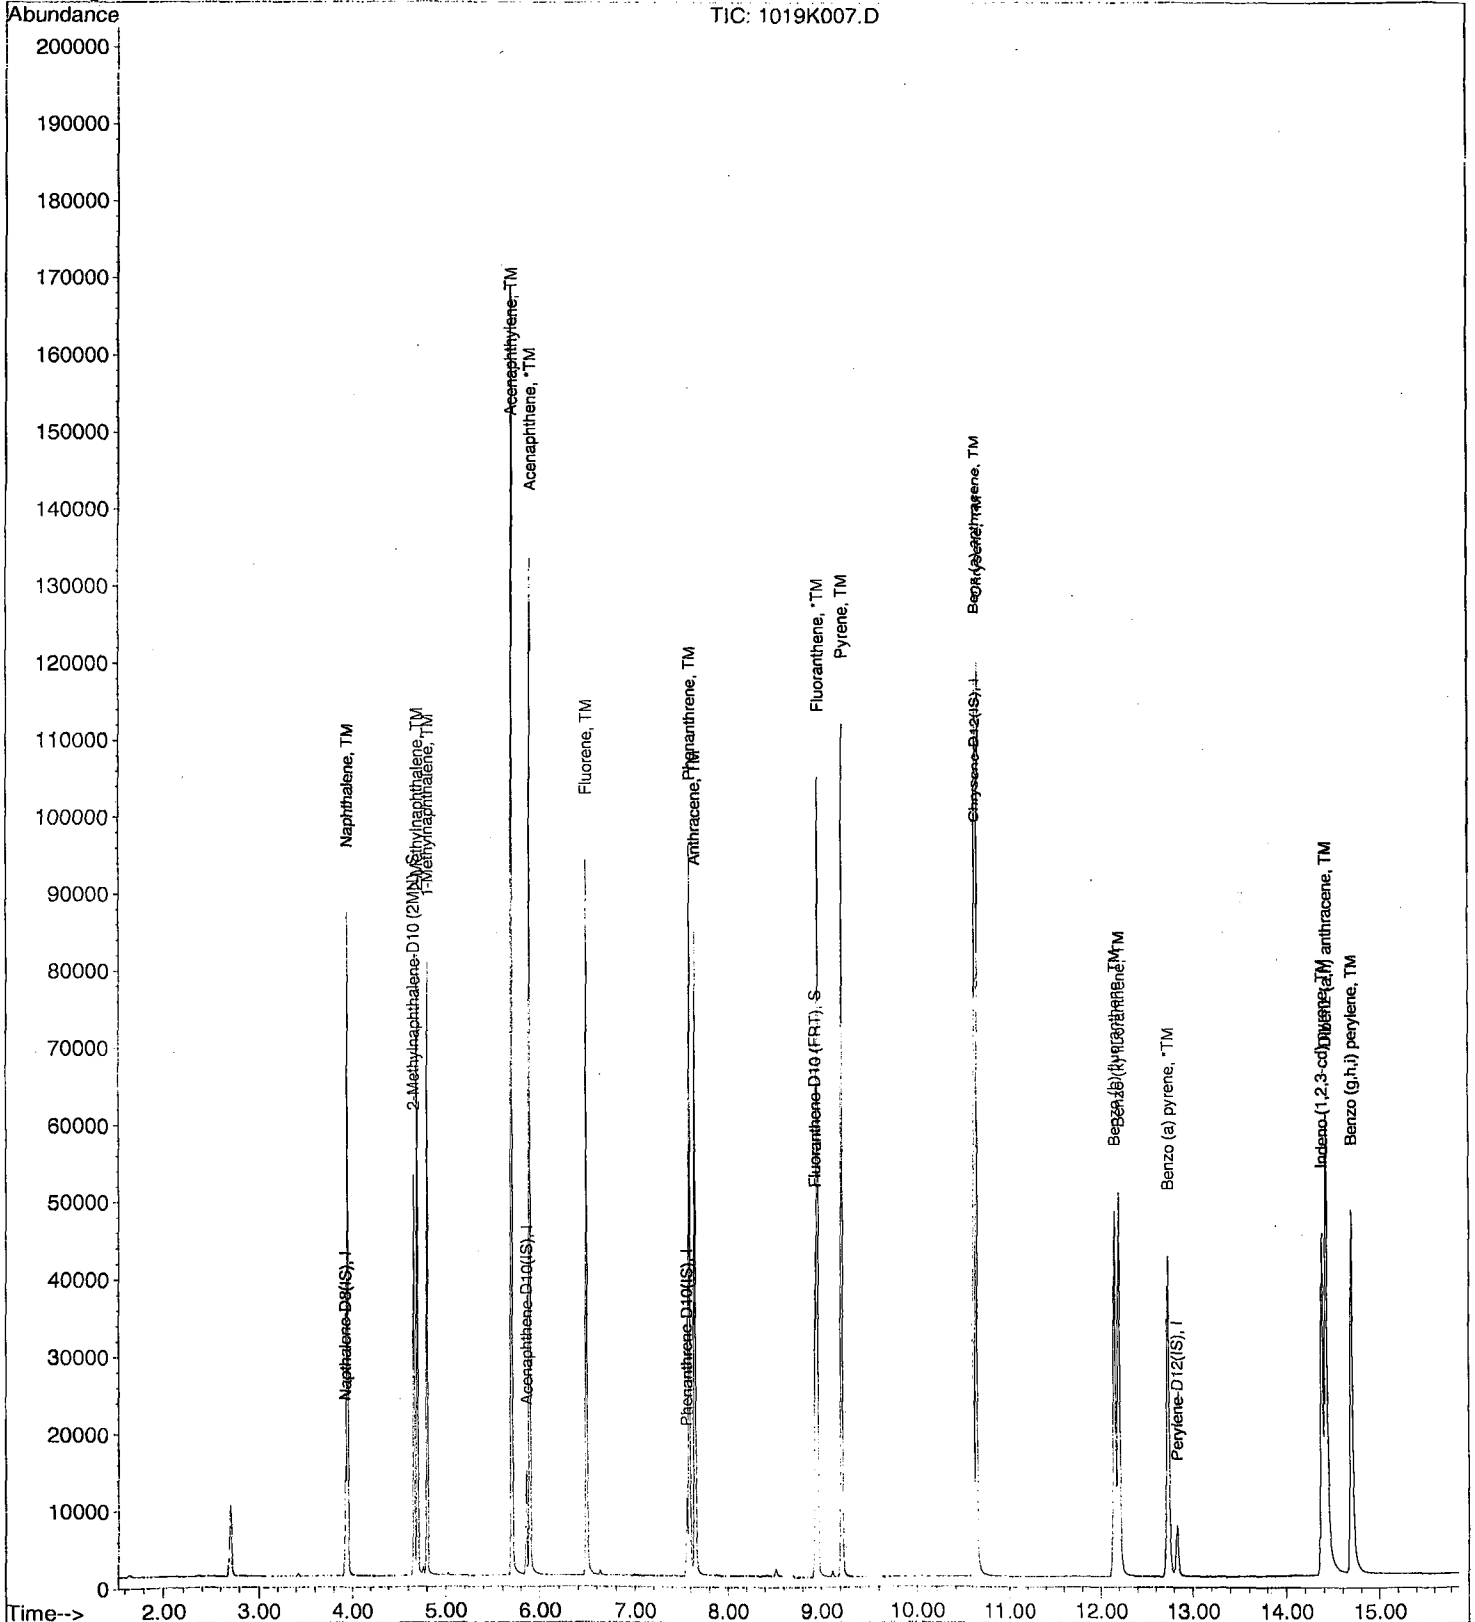

Quantitation Report (Not Reviewed)

Data File : M:\KYLO\DATA\211019\1019K008.D
 Acq On : 19 Oct 21 16:09
 Sample : 50 ug/ml 10/13/21
 Misc :

Vial: 8
 Operator: LS
 Inst : KYLO
 Multiplr: 1.00

Quant Time: Oct 19 15:49 2021

Quant Results File: K1019.RES

Quant Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)
 Title : EPA 8270
 Last Update : Tue Oct 19 16:47:23 2021
 Response via : Initial Calibration
 DataAcq Meth : SIM_2

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Napthalene-D8 (IS)	3.92	136	11542	2.50000	ppb	0.00
6) Acenaphthene-D10 (IS)	5.86	164	5767	2.50000	ppb	0.00
10) Phenanthrene-D10 (IS)	7.56	188	8902	2.50000	ppb	0.00
15) Chrysene-D12 (IS)	10.62	240	10648	2.50000	ppb	0.00
20) Perylene-D12 (IS)	12.83	264	9592	2.50000	ppb	0.00
System Monitoring Compounds						
3) 2-Methylnaphthalene-D10 (2)	4.66	152	140995	23.92178	ppb	0.00
Spiked Amount	5.000		Recovery	=	478.440%	
13) Fluoranthene-D10 (FRT)	8.93	212	173855	25.05302	ppb	0.00
Spiked Amount	5.000		Recovery	=	501.060%	
Target Compounds						
						Qvalue
2) Naphthalene	3.94	128	270597	45.13299	ppb	100
4) 2-Methylnaphthalene	4.69	142	165624	47.13496	ppb	99
5) 1-Methylnaphthalene	4.80	142	164402	46.35966	ppb	99
7) Acenaphthylene	5.70	152	560845	46.97510	ppb	100
8) Acenaphthene	5.89	154	145964	46.15736	ppb	99
9) Fluorene	6.49	166	175391	47.86199	ppb	100
11) Phenanthrene	7.59	178	233010	47.56290	ppb	100
12) Anthracene	7.64	178	228704	49.42683	ppb	100
14) Fluoranthene	8.96	202	371445	48.80706	ppb	99
16) Pyrene	9.21	202	379423	46.53971	ppb	98
17) Benz (a) anthracene	10.61	228	291856	48.90228	ppb	100
18) Chrysene	10.65	228	300277	45.25466	ppb	99
19) Indeno (1,2,3-cd) pyrene	14.38	276	248943	50.15933	ppb	94
21) Benzo (b) fluoranthene	12.15	252	294828	51.34534	ppb	99
22) Benzo (k) fluoranthene	12.20	252	302763	52.24864	ppb	100
23) Benzo (a) pyrene	12.73	252	278840	51.91758	ppb	100
24) Dibenz (a,h) anthracene	14.42	278	268409	51.28254	ppb	97
25) Benzo (g,h,i) perylene	14.70	276	280479	51.78283	ppb	99

Quantitation Report


Data File : M:\KYLO\DATA\211019\1019K008.D
Acq On : 19 Oct 21 16:09
Sample : 50 ug/ml 10/13/21
Misc :

Vial: 8
Operator: LS
Inst : KYLO
Multiplr: 1.00

Quant Time: Oct 19 15:49 2021

Quant Results File: K1019.RES

Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)
Title : EPA 8270
Last Update : Tue Nov 09 10:14:45 2021
Response via : Initial Calibration

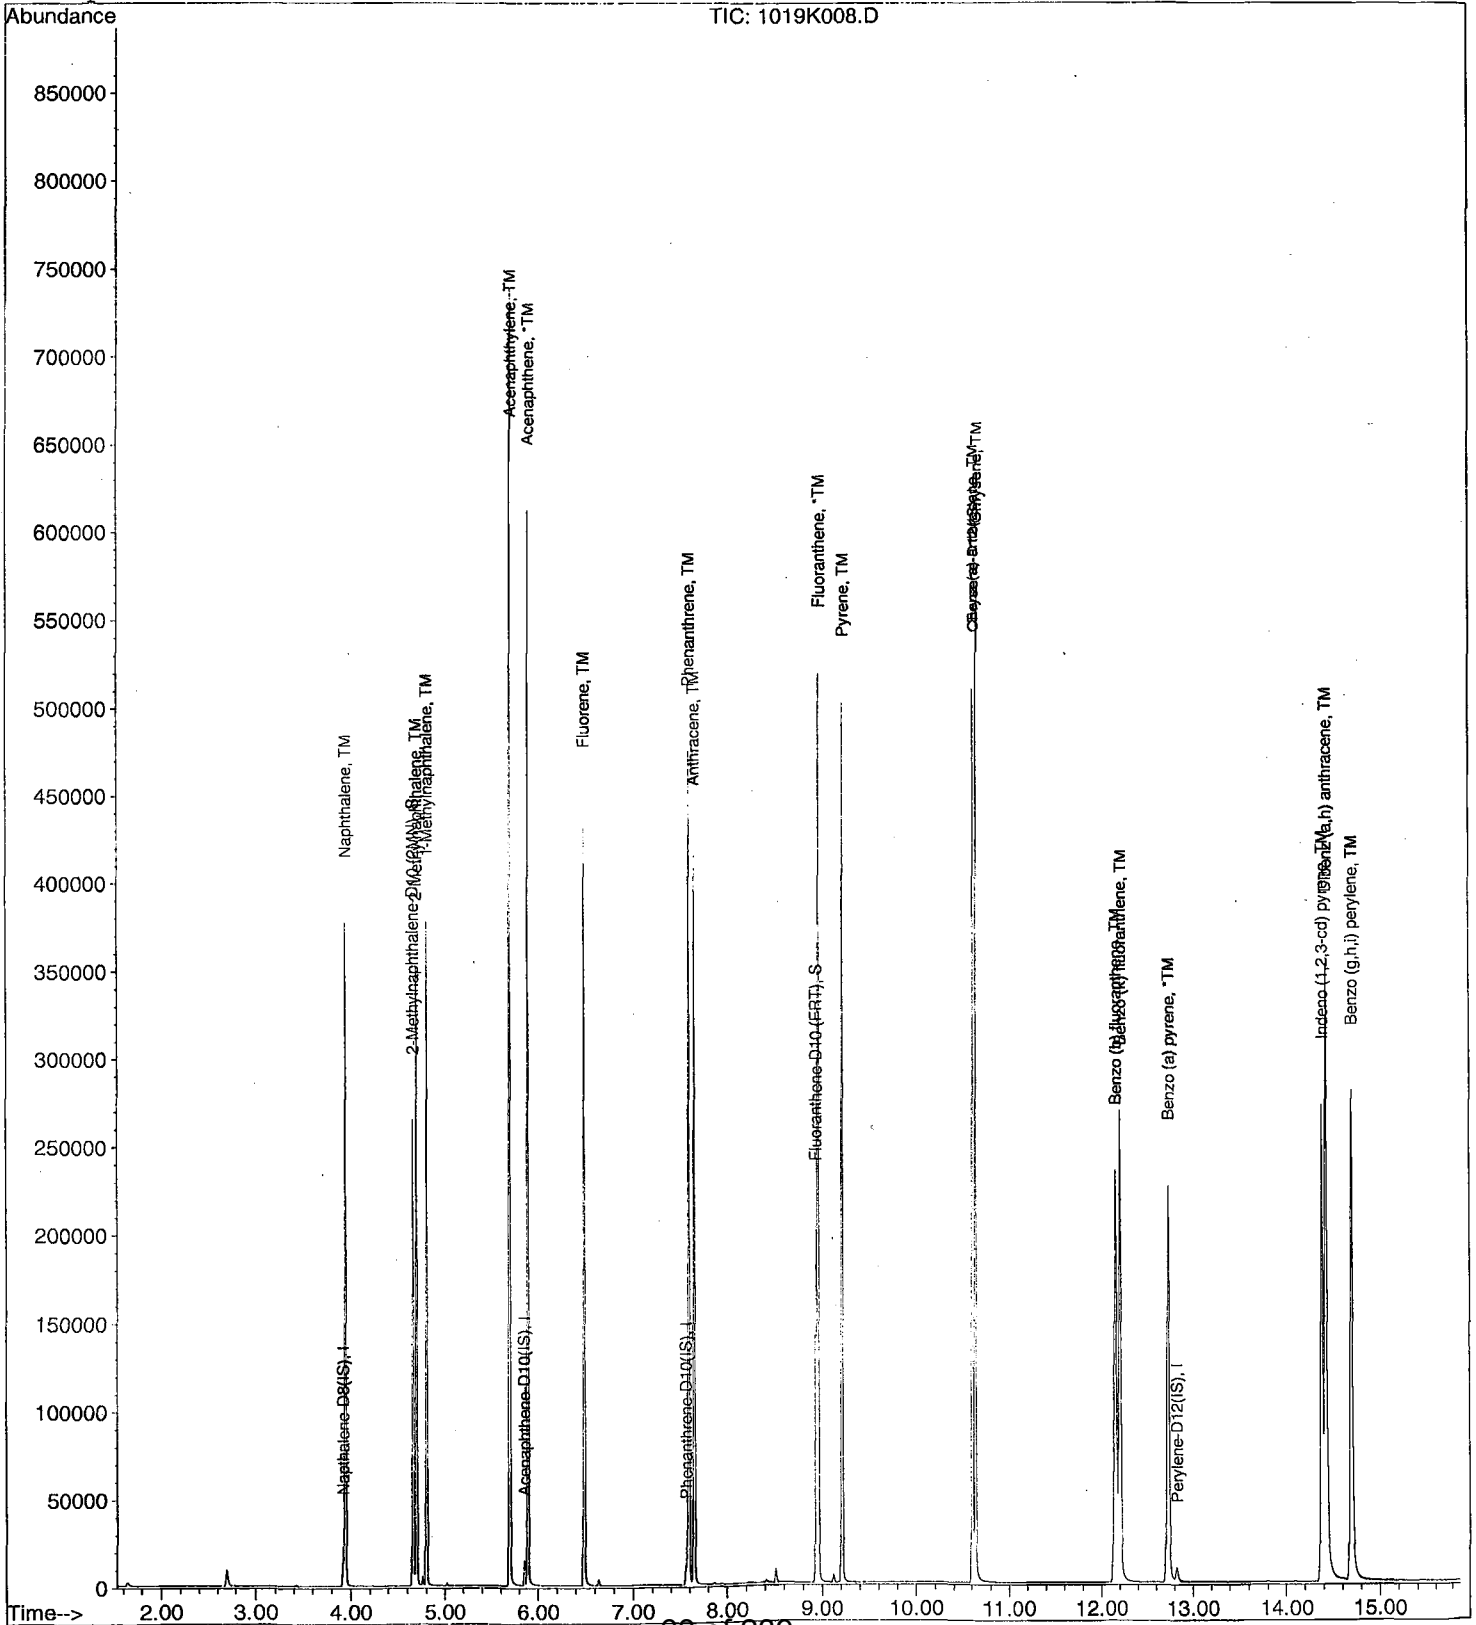

Data File : M:\KYLO\DATA\211019\1019K009.D
 Acq On : 19 Oct 21 16:29
 Sample : 100 ug/ml 10/13/21
 Misc :

Vial: 9
 Operator: LS
 Inst : KYLO
 Multiplr: 1.00

Quant Time: Oct 19 15:49 2021

Quant Results File: K1019.RES

Quant Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)
 Title : EPA 8270
 Last Update : Tue Oct 19 16:47:23 2021
 Response via : Initial Calibration
 DataAcq Meth : SIM_2

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Napthalene-D8 (IS)	3.92	136	11679	2.50000	ppb	0.00
6) Acenaphthene-D10 (IS)	5.86	164	5877	2.50000	ppb	0.00
10) Phenanthrene-D10 (IS)	7.56	188	9024	2.50000	ppb	0.00
15) Chrysene-D12 (IS)	10.63	240	10469	2.50000	ppb	0.01
20) Perylene-D12 (IS)	12.83	264	9899	2.50000	ppb	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 2-Methylnaphthalene-D10 (2)	4.66	152	278374	46.67602	ppb	0.00
Spiked Amount	5.000		Recovery	=	933.520%	
13) Fluoranthene-D10 (FRT)	8.94	212	341108	48.49012	ppb	0.00
Spiked Amount	5.000		Recovery	=	969.800%	

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Naphthalene	3.94	128	514066	84.73550	ppb	100
4) 2-Methylnaphthalene	4.70	142	318816	89.66757	ppb	99
5) 1-Methylnaphthalene	4.80	142	317528	88.48927	ppb	98
7) Acenaphthylene	5.70	152	1047512	86.09505	ppb	98
8) Acenaphthene	5.90	154	283708	88.03615	ppb	94
9) Fluorene	6.49	166	342219	91.63932	ppb	99
11) Phenanthrene	7.59	178	452383	91.09374	ppb	99
12) Anthracene	7.65	178	447639	95.43451	ppb	100
14) Fluoranthene	8.96	202	701599	90.94222	ppb	97
16) Pyrene	9.22	202	720167	89.84545	ppb	99
17) Benz (a) anthracene	10.62	228	562838	95.91946	ppb	99
18) Chrysene	10.66	228	575910	88.27926	ppb	98
19) Indeno (1,2,3-cd) pyrene	14.39	276	488982	100.01982	ppb	89
21) Benzo (b) fluoranthene	12.16	252	587997	99.33083	ppb	100
22) Benzo (k) fluoranthene	12.16	252	587786	98.78137	ppb	99
23) Benzo (a) pyrene	12.74	252	547488	99.01252	ppb	98
24) Dibenz (a,h) anthracene	14.43	278	535891	99.35185	ppb	94
25) Benzo (g,h,i) perylene	14.71	276	552068	99.06661	ppb	98

Quantitation Report


Data File : M:\KYLO\DATA\211019\1019K009.D
Acq On : 19 Oct 21 16:29
Sample : 100 ug/ml 10/13/21
Misc :

Vial: 9
Operator: LS
Inst : KYLO
Multiplr: 1.00

Quant Time: Oct 19 15:49 2021

Quant Results File: K1019.RES

Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)
Title : EPA 8270
Last Update : Tue Nov 09 10:14:45 2021
Response via : Initial Calibration

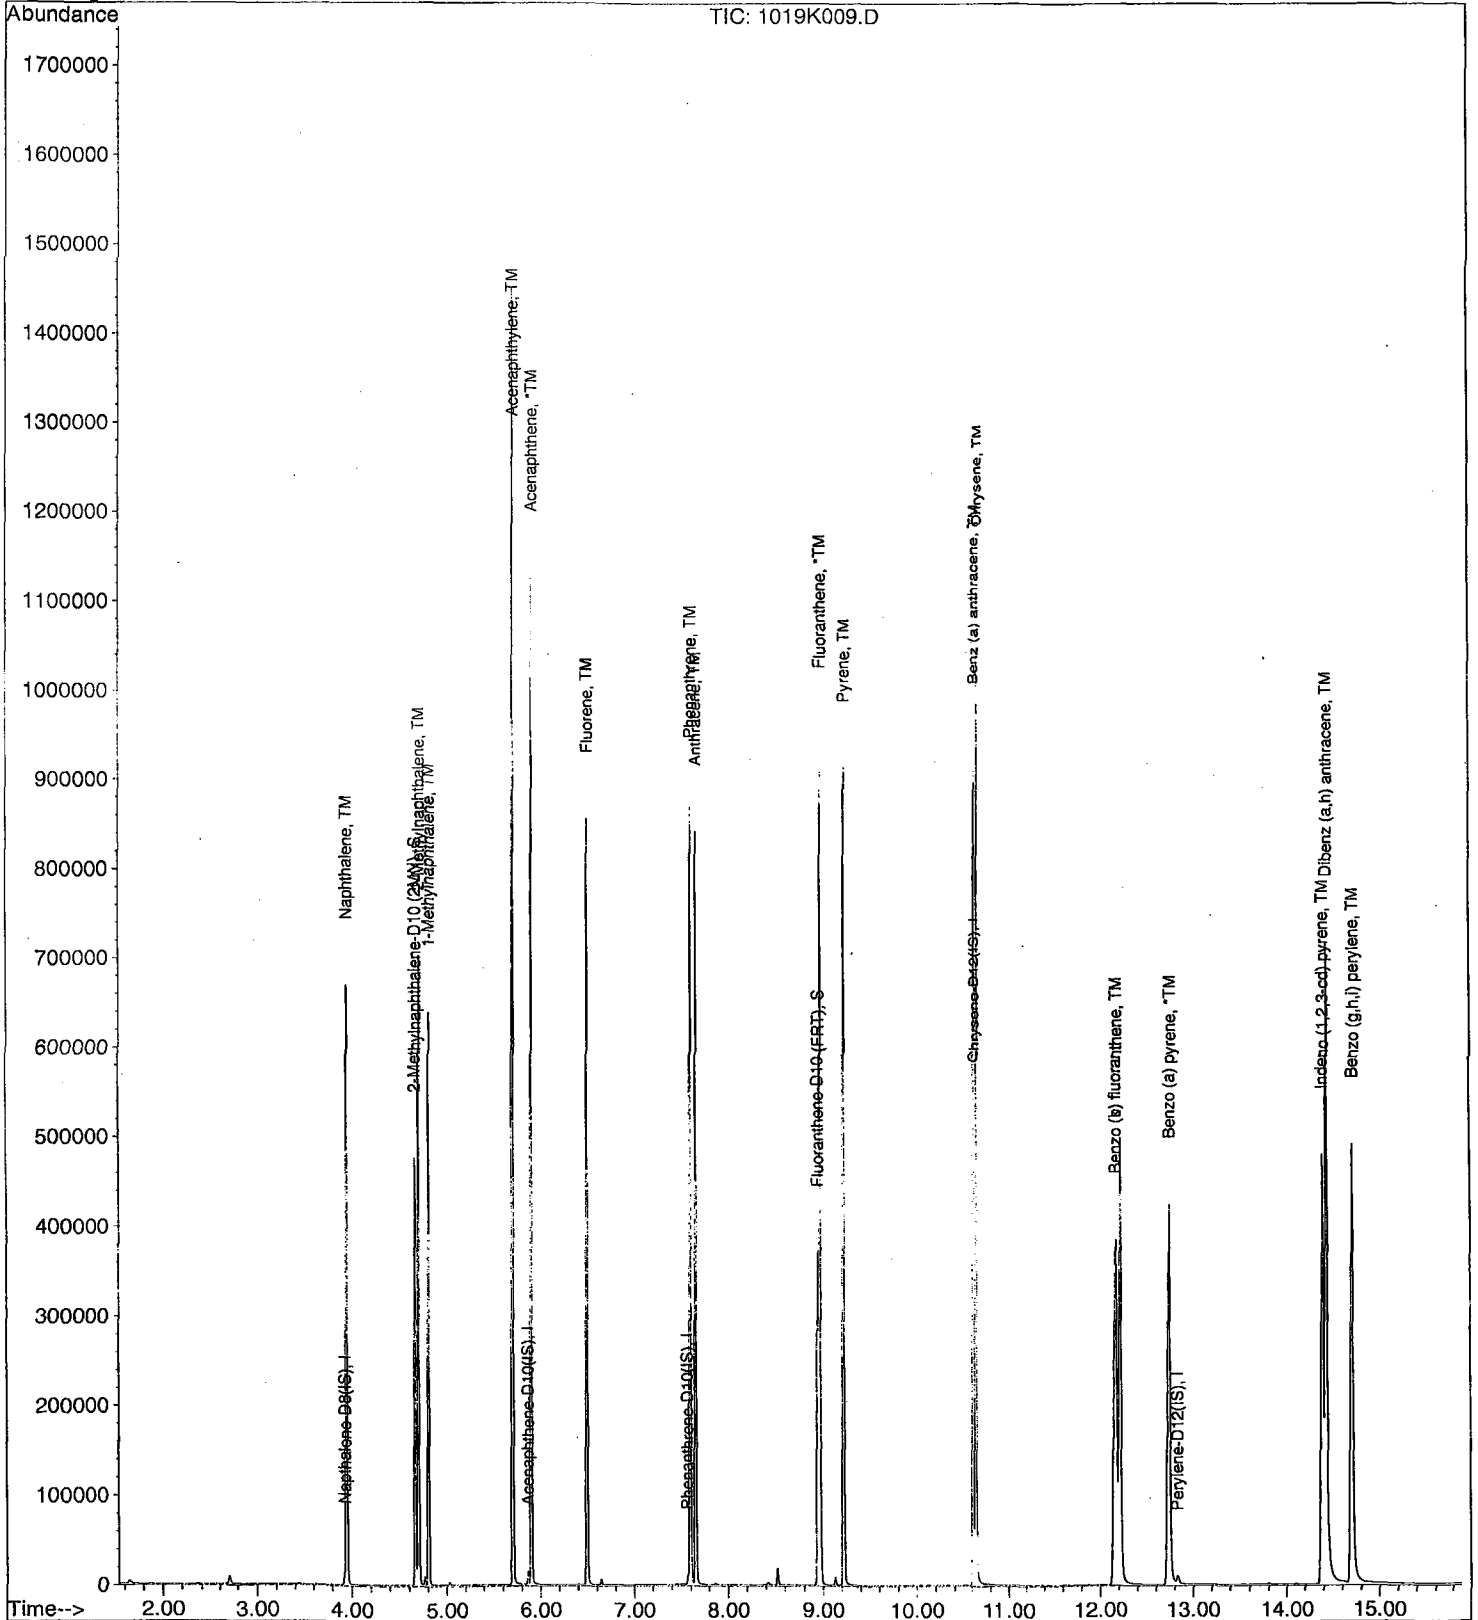

PAH by GCMS SIM
EPA 8270 SIM

Form 7

Second Source Calibration

Lab Name: APPL, Inc.
Case No: _____
Matrix: _____

SDG No: _____
Date Analyzed: 10/19/2021
Instrument: KYLO
Initial Cal. Date: 10/19/2021
Data File: 1019K010.D

		Compound	MEAN	CCRF	%D	%Drift
1	TM	Naphthalene	1.299	1.295	0.25	TM
2	TM	2-Methylnaphthalene	0.7611	0.7635	0.32	TM
3	TM	1-Methylnaphthalene	0.7681	0.7563	1.5	TM
4	TM	Acenaphthylene	5.176	5.272	1.9	TM
5	*TM	Acenaphthene	1.371	1.393	1.6	*TM
6	TM	Fluorene	1.589	1.616	1.7	TM
7	TM	Phenanthrene	1.376	1.380	0.31	TM
8	TM	Anthracene	1.299	1.415	8.9	TM
9	*TM	Fluoranthene	2.137	2.167	1.4	*TM
10	TM	Pyrene	1.914	1.918	0.21	TM
11	TM	Benz (a) anthracene	1.401	1.374	1.9	TM
12	TM	Chrysene	1.558	1.488	4.5	TM
13	TML	Indeno (1,2,3-cd) pyrene	1.272	0.9799	23	TML 12
14	TM	Benzo (b) fluoranthene	1.408	1.510	7.3	TM
15	TM	Benzo (k) fluoranthene	1.610	1.698	5.5	TM
16	*TM	Benzo (a) pyrene	1.341	1.484	11	*TM
17	TM	Dibenz (a,h) anthracene	1.326	1.382	4.2	TM
18	TM	Benzo (g,h,i) perylene	1.443	1.486	3.0	TM
19						
20						
21						
22						
23						
24						
25						
26						
27						
28						
29						
30						
31						
32						
33						
34						
35						
36						
37						
38						

Average

4.4

PAH by GCMS SIM
EPA 8270 SIM

Quantitation Report (Not Reviewed)

Data File : M:\KYLO\DATA\211019\1019K010.D
 Acq On : 19 Oct 21 16:49
 Sample : SS ug/ml 10/13/21
 Misc :

Vial: 10
 Operator: LS
 Inst : KYLO
 Multiplr: 1.00

Quant Time: Oct 19 16:06 2021

Quant Results File: K1019.RES

Quant Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)
 Title : EPA 8270
 Last Update : Tue Oct 19 16:51:19 2021
 Response via : Initial Calibration
 DataAcq Meth : SIM_2

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Napthalene-D8 (IS)	3.92	136	11540	2.50000	ppb	0.00
6) Acenaphthene-D10 (IS)	5.86	164	5722	2.50000	ppb	0.00
10) Phenanthrene-D10 (IS)	7.56	188	8843	2.50000	ppb	0.00
15) Chrysene-D12 (IS)	10.62	240	10394	2.50000	ppb	0.00
20) Perylene-D12 (IS)	12.83	264	8800	2.50000	ppb	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 2-Methylnaphthalene-D10 (2)	4.66	152	1	0.00017	ppb	0.00
Spiked Amount	5.000		Recovery	=	0.000%	
13) Fluoranthene-D10 (FRT)	8.93	212	9	0.00131	ppb	0.00
Spiked Amount	5.000		Recovery	=	0.020%	

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Naphthalene	3.94	128	29897	4.98740	ppb	100
4) 2-Methylnaphthalene	4.69	142	17622	5.01592	ppb	100
5) 1-Methylnaphthalene	4.80	142	17455	4.92298	ppb	100
7) Acenaphthylene	5.69	152	60338	5.09352	ppb	100
8) Acenaphthene	5.89	154	15936	5.07898	ppb	100
9) Fluorene	6.49	166	18488	5.08482	ppb	100
11) Phenanthrene	7.59	178	24407	5.01529	ppb	100
12) Anthracene	7.64	178	25019	5.44311	ppb	100
14) Fluoranthene	8.95	202	38328	5.06982	ppb	99
16) Pyrene	9.21	202	39873	5.01031	ppb	100
17) Benz (a) anthracene	10.61	228	28567	4.90355	ppb	99
18) Chrysene	10.65	228	30939	4.77675	ppb	100
19) Indeno (1,2,3-cd) pyrene	14.38	276	20371	4.37871	ppb	99
21) Benzo (b) fluoranthene	12.14	252	26577	5.36265	ppb	100
22) Benzo (k) fluoranthene	12.19	252	29888	5.27373	ppb	100
23) Benzo (a) pyrene	12.73	252	26127	5.53492	ppb	100
24) Dibenz (a,h) anthracene	14.42	278	24324	5.21145	ppb	99
25) Benzo (g,h,i) perylene	14.69	276	26159	5.14999	ppb	100

Quantitation Report


Data File : M:\KYLO\DATA\211019\1019K010.D
Acq On : 19 Oct 21 16:49
Sample : SS ug/ml 10/13/21
Misc :

Vial: 10
Operator: LS
Inst : KYLO
Multiplr: 1.00

Quant Time: Oct 19 16:06 2021

Quant Results File: K1019.RES

Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)
Title : EPA 8270
Last Update : Tue Nov 09 10:14:45 2021
Response via : Initial Calibration

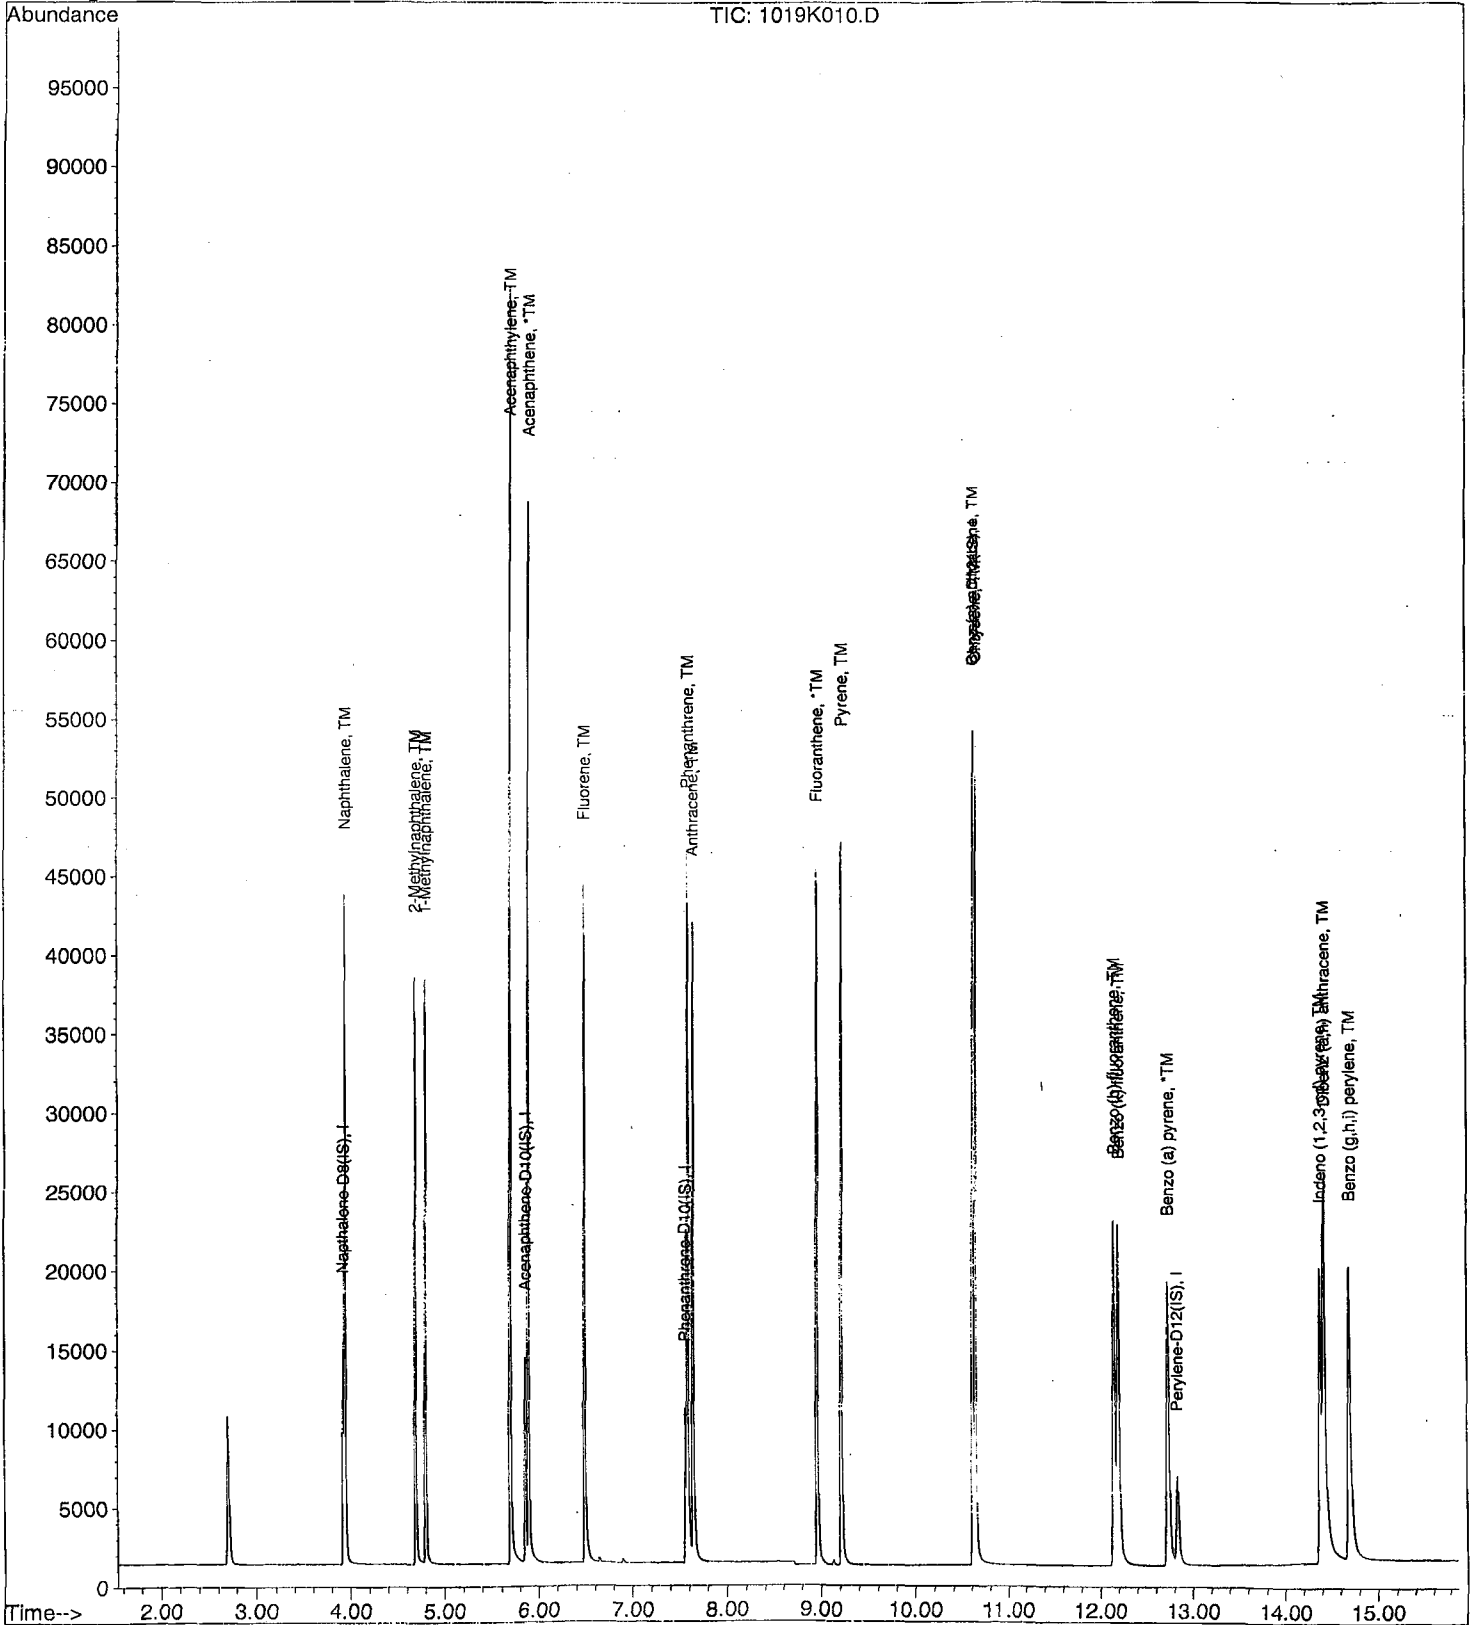

PAH by GCMS SIM
EPA 8270 SIM

Form 7

Continuing Calibration

Lab Name: APPL, Inc.

SDG No: _____

Case No: _____

Date Analyzed: 10/28/2021

Matrix: _____

Instrument: KYLO

Initial Cal. Date: 10/19/2021

Data File: 1019K171.D

		Compound	MEAN	CCRF	%D	%Drift
1	I	Naphthalene-D8(IS)	ISTD			I
2	TM	Naphthalene	1.299	1.327	2.2	TM
3	S	2-Methylnaphthalene-D10 (2MN)	1.277	1.294	1.3	S
4	TM	2-Methylnaphthalene	0.7611	0.8077	6.1	TM
5	TM	1-Methylnaphthalene	0.7681	0.8019	4.4	TM
6	I	Acenaphthene-D10(IS)	ISTD			I
7	TM	Acenaphthylene	5.176	5.448	5.3	TM
8	*TM	Acenaphthene	1.371	1.423	3.8	*TM
9	TM	Fluorene	1.589	1.678	5.7	TM
10	I	Phenanthrene-D10(IS)	ISTD			I
11	TM	Phenanthrene	1.376	1.470	6.8	TM
12	TM	Anthracene	1.299	1.377	6.0	TM
13	S	Fluoranthene-D10 (FRT)	1.949	1.989	2.1	S
14	*TM	Fluoranthene	2.137	2.351	10.0	*TM
15	I	Chrysene-D12(IS)	ISTD			I
16	TM	Pyrene	1.914	1.991	4.0	TM
17	TM	Benz (a) anthracene	1.401	1.479	5.5	TM
18	TM	Chrysene	1.558	1.563	0.32	TM
19	TML	Indeno (1,2,3-cd) pyrene	1.272	1.117	12	TML 0.74
20	I	Perylene-D12(IS)	ISTD			I
21	TM	Benzo (b) fluoranthene	1.408	1.570	11	TM
22	TM	Benzo (k) fluoranthene	1.610	1.696	5.4	TM
23	*TM	Benzo (a) pyrene	1.341	1.456	8.6	*TM
24	TM	Dibenz (a,h) anthracene	1.326	1.393	5.0	TM
25	TM	Benzo (g,h,i) perylene	1.443	1.557	7.9	TM
26						
27						
28						
29						
30						
31						
32						
33						
34						
35						
36						
37						
38						
39						
40						

Average

5.7

Quantitation Report (Not Reviewed)

Data File : M:\KYLO\DATA\211019\1019K171.D
 Acq On : 28 Oct 21 9:18
 Sample : 5 ug/ml 10/19/21 (1)
 Misc :

Vial: 21
 Operator: LS
 Inst : KYLO
 Multiplr: 1.00

Quant Time: Oct 28 8:38 2021

Quant Results File: K1019.RES

Quant Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)

Title : EPA 8270
 Last Update : Wed Oct 27 10:57:36 2021
 Response via : Initial Calibration
 DataAcq Meth : SIM_2

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Naphthalene-D8 (IS)	3.89	136	13064	2.50	ppb	0.00
6) Acenaphthene-D10 (IS)	5.82	164	6432	2.50	ppb	-0.03
10) Phenanthrene-D10 (IS)	7.52	188	9841	2.50	ppb	-0.03
15) Chrysene-D12 (IS)	10.58	240	11899	2.50	ppb	-0.04
20) Perylene-D12 (IS)	12.76	264	10623	2.50	ppb	-0.07
System Monitoring Compounds						
3) 2-Methylnaphthalene-D10 (2)	4.63	152	16903	2.53	ppb	-0.03
Spiked Amount	5.000		Recovery	=	50.680%	
13) Fluoranthene-D10 (FRT)	8.90	212	19572	2.55	ppb	-0.03
Spiked Amount	5.000		Recovery	=	51.020%	
Target Compounds						
2) Naphthalene	3.91	128	34671	5.11	ppb	100
4) 2-Methylnaphthalene	4.66	142	21104	5.31	ppb	98
5) 1-Methylnaphthalene	4.77	142	20953	5.22	ppb	98
7) Acenaphthylene	5.66	152	70079	5.26	ppb	99
8) Acenaphthene	5.86	154	18309	5.19	ppb	97
9) Fluorene	6.45	166	21591	5.28	ppb	99
11) Phenanthrene	7.55	178	28931	5.34	ppb	100
12) Anthracene	7.61	178	27111	5.30	ppb	100
14) Fluoranthene	8.92	202	46263	5.50	ppb	96
16) Pyrene	9.18	202	47381	5.20	ppb	95
17) Benz (a) anthracene	10.57	228	35190	5.28	ppb	99
18) Chrysene	10.61	228	37193	5.02	ppb	99
19) Indeno (1,2,3-cd) pyrene	14.32	276	26574	4.96	ppb	95
21) Benzo (b) fluoranthene	12.08	252	33346	5.57	ppb	99
22) Benzo (k) fluoranthene	12.13	252	36038	5.27	ppb	98
23) Benzo (a) pyrene	12.66	252	30944	5.43	ppb	99
24) Dibenz (a,h) anthracene	14.37	278	29588	5.25	ppb	100
25) Benzo (g,h,i) perylene	14.64	276	33088	5.40	ppb	99

Quantitation Report


Data File : M:\KYLO\DATA\211019\1019K171.D
Acq On : 28 Oct 21 9:18
Sample : 5 ug/ml 10/19/21 (1)
Misc :

Vial: 21
Operator: LS
Inst : KYLO
Multiplr: 1.00

Quant Time: Oct 28 8:38 2021

Quant Results File: K1019.RES

Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)
Title : EPA 8270
Last Update : Tue Nov 09 10:14:45 2021
Response via : Initial Calibration

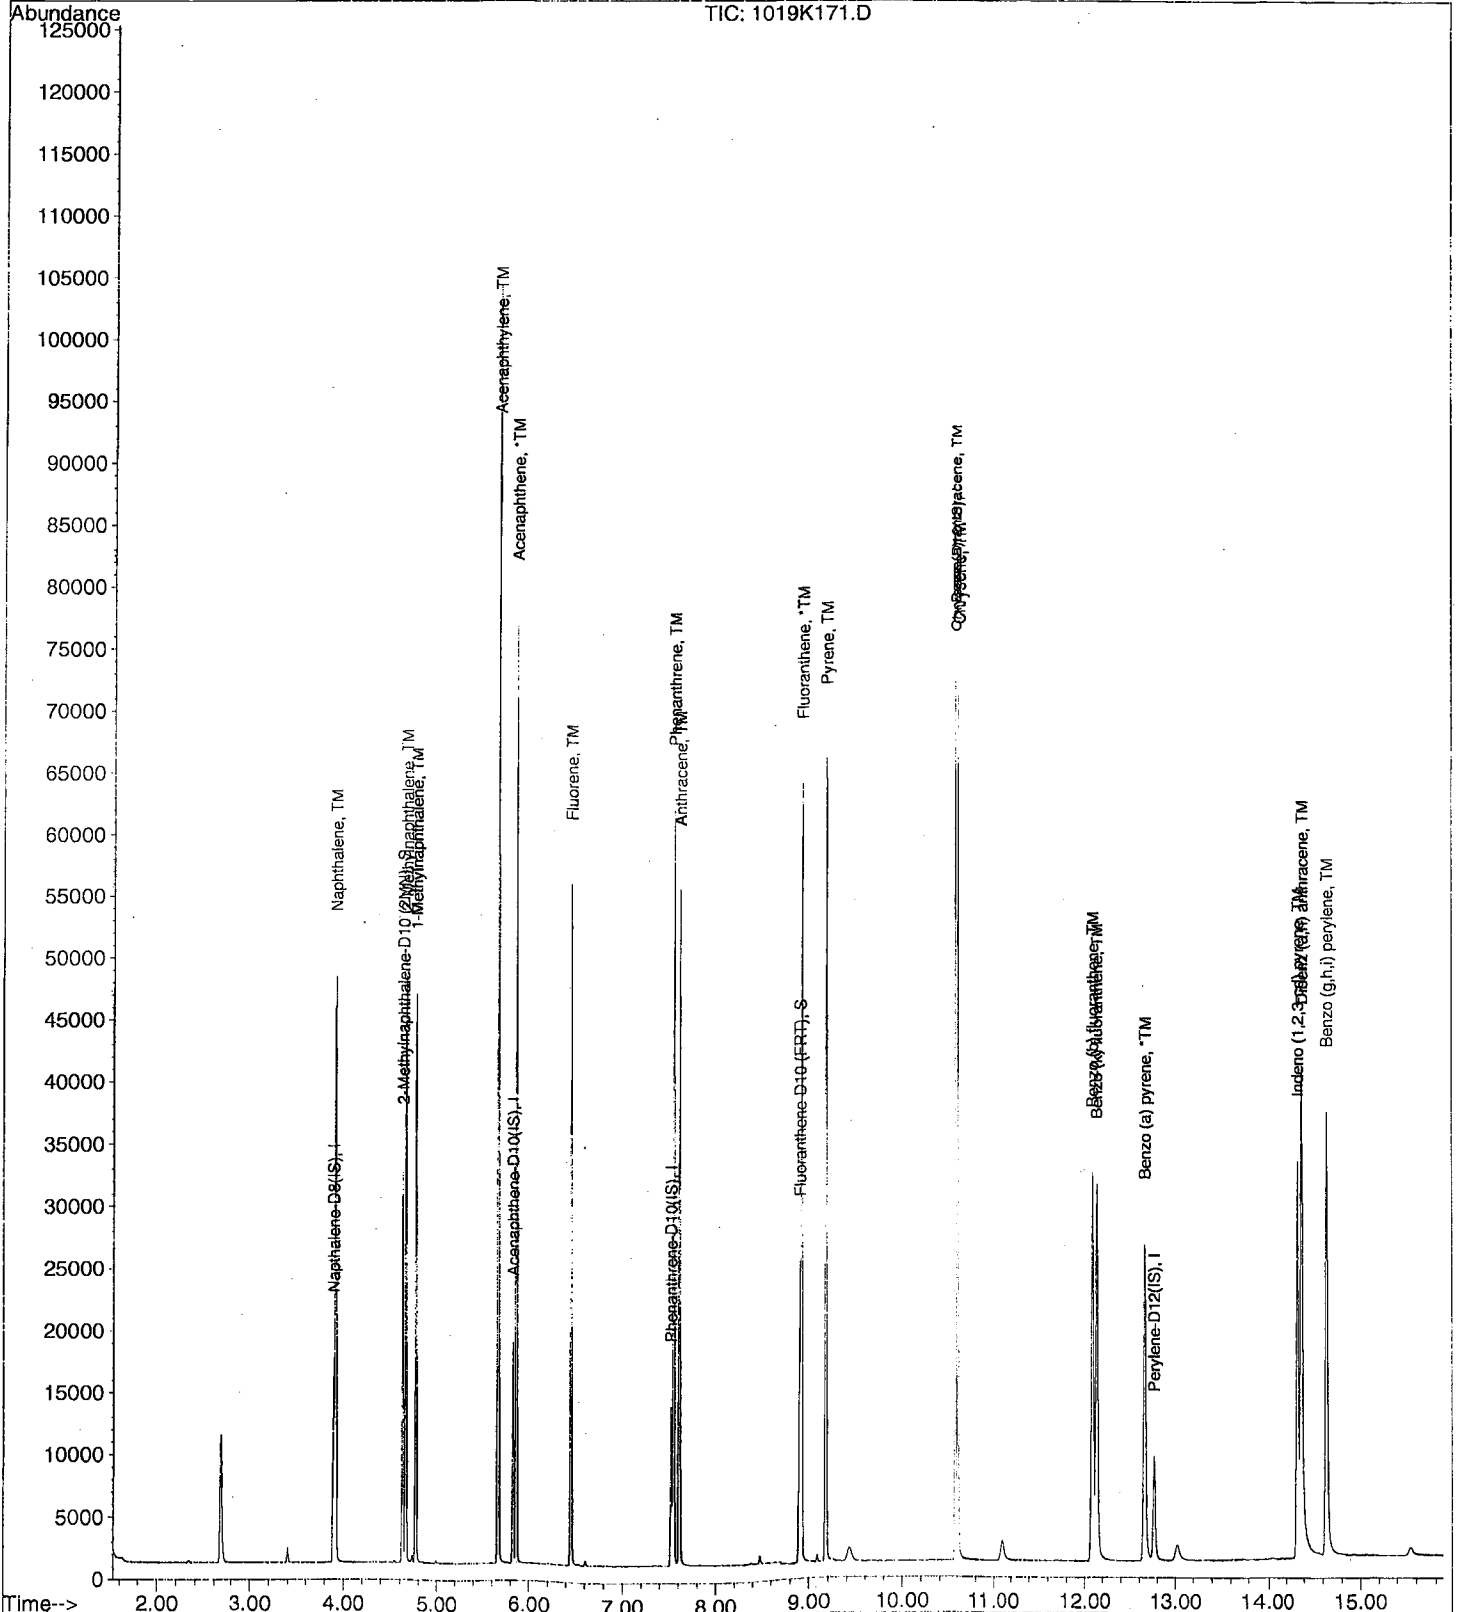

PAH by GCMS SIM
EPA 8270 SIM

Form 7

Ending Continuing Calibration

Lab Name: APPL, Inc.
Case No: _____
Matrix: _____

SDG No: _____
Date Analyzed: 10/28/2021
Instrument: KYLO
Initial Cal. Date: 10/19/2021
Data File: 1019K205.D

		Compound	MEAN	CCRF	%D	%Drift
1	I	Napthalene-D8(IS)	ISTD			I
2	TM	Napthalene	1.299	1.305	0.45	TM
3	S	2-Methylnapthalene-D10 (2MN)	1.277	1.287	0.79	S
4	TM	2-Methylnapthalene	0.7611	0.8002	5.1	TM
5	TM	1-Methylnapthalene	0.7681	0.7954	3.6	TM
6	I	Acenaphthene-D10(IS)	ISTD			I
7	TM	Acenaphthylene	5.176	5.292	2.3	TM
8	*TM	Acenaphthene	1.371	1.405	2.5	*TM
9	TM	Fluorene	1.589	1.663	4.7	TM
10	I	Phenanthrene-D10(IS)	ISTD			I
11	TM	Phenanthrene	1.376	1.447	5.2	TM
12	TM	Anthracene	1.299	1.356	4.4	TM
13	S	Fluoranthene-D10 (FRT)	1.949	2.068	6.1	S
14	*TM	Fluoranthene	2.137	2.304	7.8	*TM
15	I	Chrysene-D12(IS)	ISTD			I
16	TM	Pyrene	1.914	1.977	3.3	TM
17	TM	Benz (a) anthracene	1.401	1.480	5.6	TM
18	TM	Chrysene	1.558	1.545	0.83	TM
19	TML	Indeno (1,2,3-cd) pyrene	1.272	1.089	14	TML 3.1
20	I	Perylene-D12(IS)	ISTD			I
21	TM	Benzo (b) fluoranthene	1.408	1.526	8.4	TM
22	TM	Benzo (k) fluoranthene	1.610	1.679	4.3	TM
23	*TM	Benzo (a) pyrene	1.341	1.425	6.3	*TM
24	TM	Dibenz (a,h) anthracene	1.326	1.344	1.4	TM
25	TM	Benzo (g,h,i) perylene	1.443	1.471	2.0	TM
26						
27						
28						
29						
30						
31						
32						
33						
34						
35						
36						
37						
38						
39						
40						

Average

4.5

Data File : M:\KYLO\DATA\211019\1019K205.D
 Acq On : 28 Oct 21 20:55
 Sample : 5 ug/ml 10/13/21 (2)
 Misc :

Vial: 55
 Operator: LS
 Inst : KYLO
 Multiplr: 1.00

Quant Time: Oct 29 6:36 2021

Quant Results File: K1019.RES

Quant Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)

Title : EPA 8270
 Last Update : Wed Oct 27 10:57:36 2021
 Response via : Initial Calibration
 DataAcq Meth : SIM_2

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Napthalene-D8 (IS)	3.89	136	17438	2.50000	ppb	0.00
6) Acenaphthene-D10 (IS)	5.82	164	8754	2.50000	ppb	-0.03
10) Phenanthrene-D10 (IS)	7.52	188	13434	2.50000	ppb	-0.03
15) Chrysene-D12 (IS)	10.57	240	16058	2.50000	ppb	-0.04
20) Perylene-D12 (IS)	12.76	264	14486	2.50000	ppb	-0.07

System Monitoring Compounds

3) 2-Methylnaphthalene-D10 (2)	4.63	152	22438	2.51975	ppb	-0.03
Spiked Amount	5.000		Recovery	=	50.400%	
13) Fluoranthene-D10 (FRT)	8.90	212	27776	2.65231	ppb	-0.04
Spiked Amount	5.000		Recovery	=	53.040%	

Target Compounds

	R.T.	QIon	Response	Conc	Units	Qvalue
2) Naphthalene	3.91	128	45496	5.02260	ppb	100
4) 2-Methylnaphthalene	4.66	142	27909	5.25713	ppb	99
5) 1-Methylnaphthalene	4.77	142	27740	5.17755	ppb	98
7) Acenaphthylene	5.66	152	92661	5.11288	ppb	99
8) Acenaphthene	5.86	154	24599	5.12455	ppb	99
9) Fluorene	6.45	166	29124	5.23574	ppb	100
11) Phenanthrene	7.55	178	38875	5.25831	ppb	99
12) Anthracene	7.61	178	36439	5.21840	ppb	99
14) Fluoranthene	8.92	202	61894	5.38913	ppb	100
16) Pyrene	9.17	202	63487	5.16370	ppb	98
17) Benz (a) anthracene	10.56	228	47524	5.28020	ppb	100
18) Chrysene	10.61	228	49619	4.95868	ppb	99
19) Indeno (1,2,3-cd) pyrene	14.31	276	34981	4.84580	ppb	93
21) Benzo (b) fluoranthene	12.08	252	44210	5.41911	ppb	100
22) Benzo (k) fluoranthene	12.12	252	48649	5.21470	ppb	99
23) Benzo (a) pyrene	12.66	252	41283	5.31284	ppb	100
24) Dibenz (a,h) anthracene	14.36	278	38952	5.06976	ppb	99
25) Benzo (g,h,i) perylene	14.63	276	42626	5.09793	ppb	100

Quantitation Report


Data File : M:\KYLO\DATA\211019\1019K205.D
 Acq On : 28 Oct 21 20:55
 Sample : 5 ug/ml 10/13/21 (2)
 Misc :

Vial: 55
 Operator: LS
 Inst : KYLO
 Multiplr: 1.00

Quant Time: Oct 29 6:36 2021

Quant Results File: K1019.RES

Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)
 Title : EPA 8270
 Last Update : Tue Nov 09 10:14:45 2021
 Response via : Initial Calibration

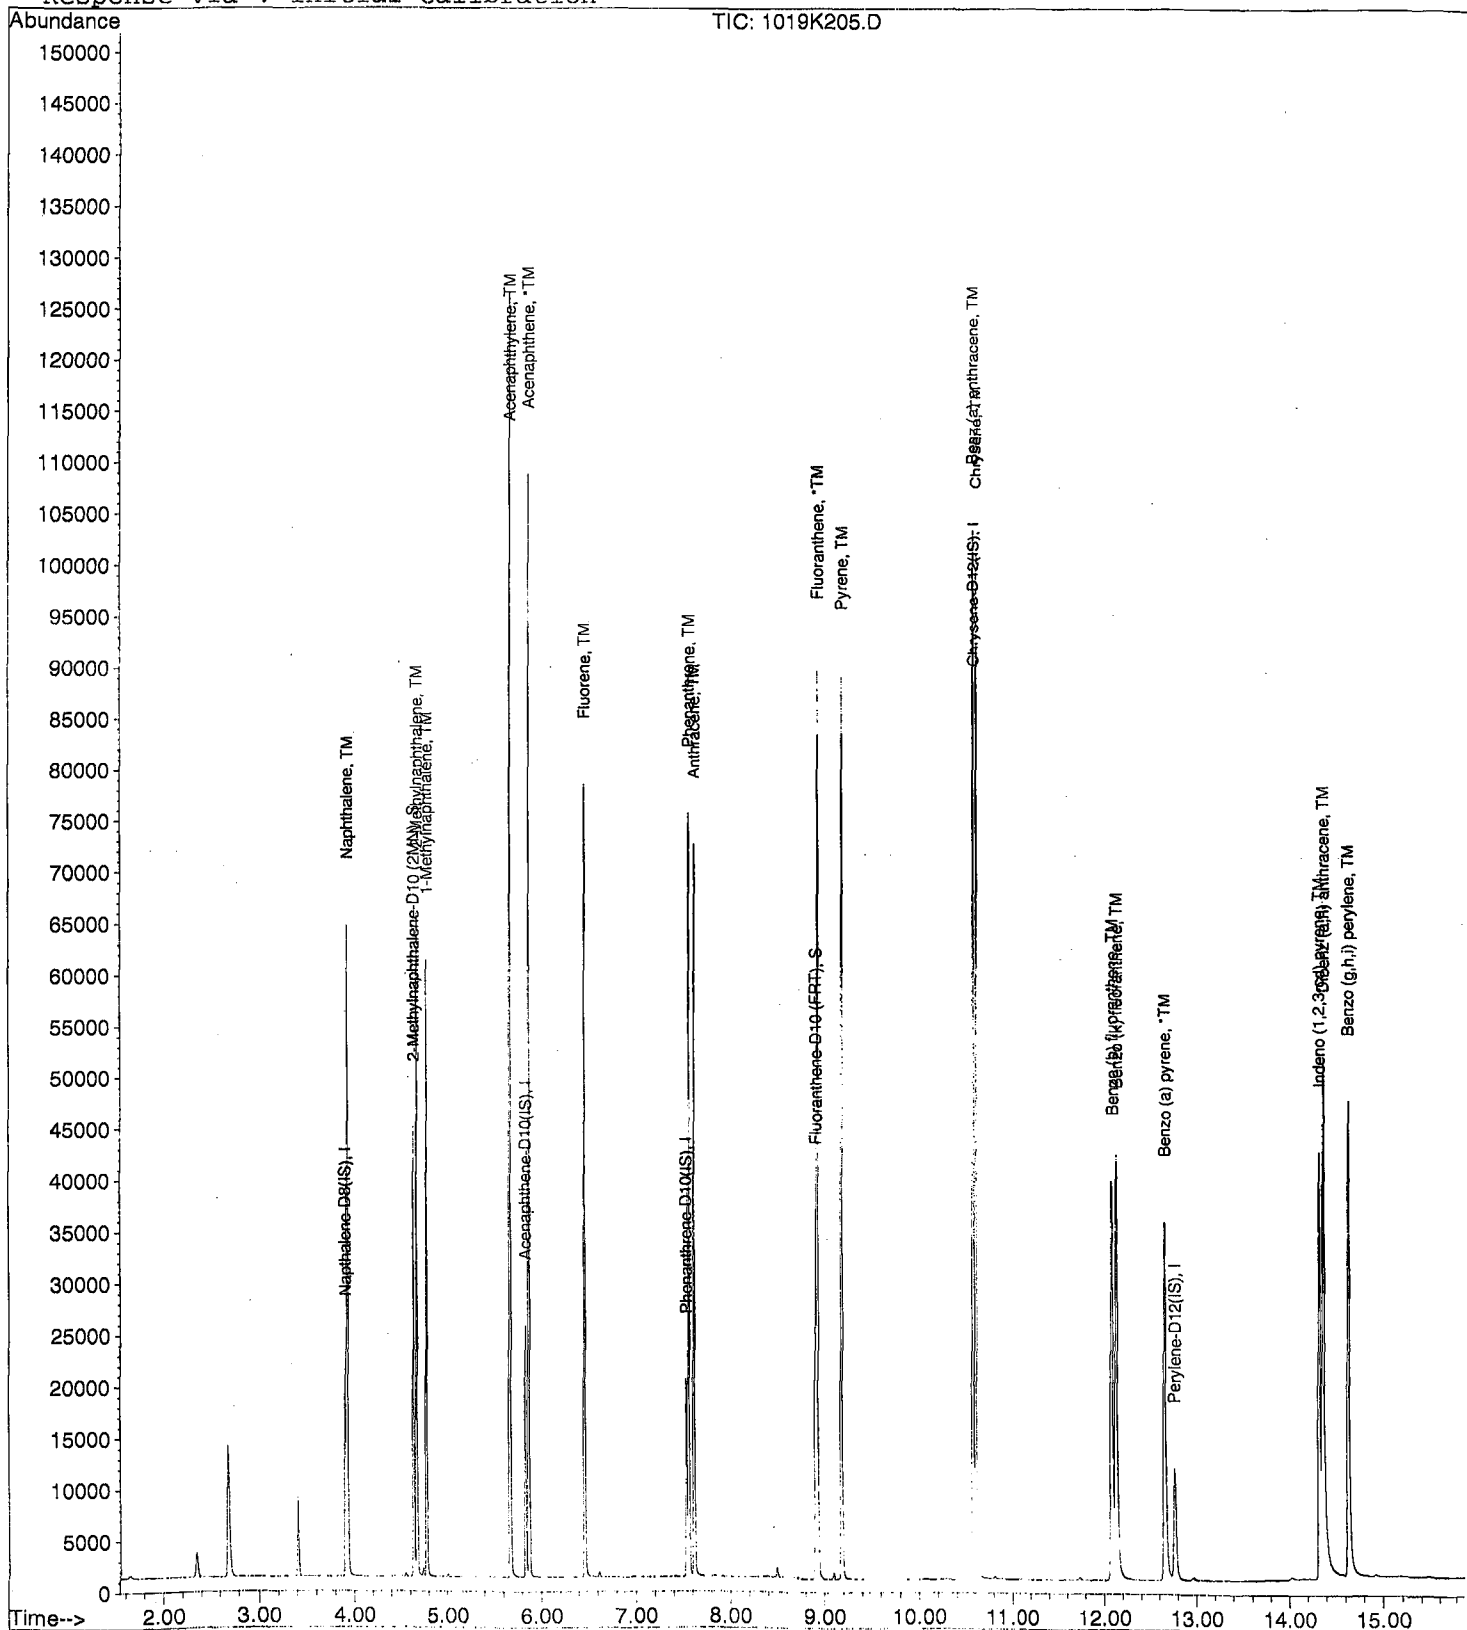

ORGANICS
Raw Data

Quantitation Report (QT Reviewed)

Data File : M:\KYLO\DATA\211019\1019K178.D Vial: 28
 Acq On : 28 Oct 21 11:55 Operator: LS
 Sample : BA43837W07 1/1000 Inst : KYLO
 Misc : Multiplr: 1.00

Quant Time: Nov 8 15:45 2021 Quant Results File: K1019.RES

Quant Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)
 Title : EPA 8270
 Last Update : Wed Oct 27 10:57:36 2021
 Response via : Initial Calibration
 DataAcq Meth : SIM_2

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Napthalene-D8 (IS)	3.89	136	13701	2.50	ppb	0.00
6) Acenaphthene-D10 (IS)	5.82	164	6820	2.50	ppb	-0.03
10) Phenanthrene-D10 (IS)	7.52	188	10379	2.50	ppb	-0.03
15) Chrysene-D12 (IS)	10.57	240	12461	2.50	ppb	-0.04
20) Perylene-D12 (IS)	12.76	264	10884	2.50	ppb	-0.07

System Monitoring Compounds						
3) 2-Methylnaphthalene-D10 (2)	4.63	152	27363	3.91	ppb	-0.03
Spiked Amount	5.000		Recovery	=	78.220%	
13) Fluoranthene-D10 (FRT)	8.90	212	32519	4.02	ppb	-0.04
Spiked Amount	5.000		Recovery	=	80.380%	

Target Compounds Qvalue

Quantitation Report


Data File : M:\KYLO\DATA\211019\1019K178.D
Acq On : 28 Oct 21 11:55
Sample : BA43837W07 1/1000
Misc :

Vial: 28
Operator: LS
Inst : KYLO
Multiplr: 1.00

Quant Time: Nov 8 15:45 2021

Quant Results File: K1019.RES

Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)
Title : EPA 8270
Last Update : Tue Nov 09 10:14:45 2021
Response via : Initial Calibration

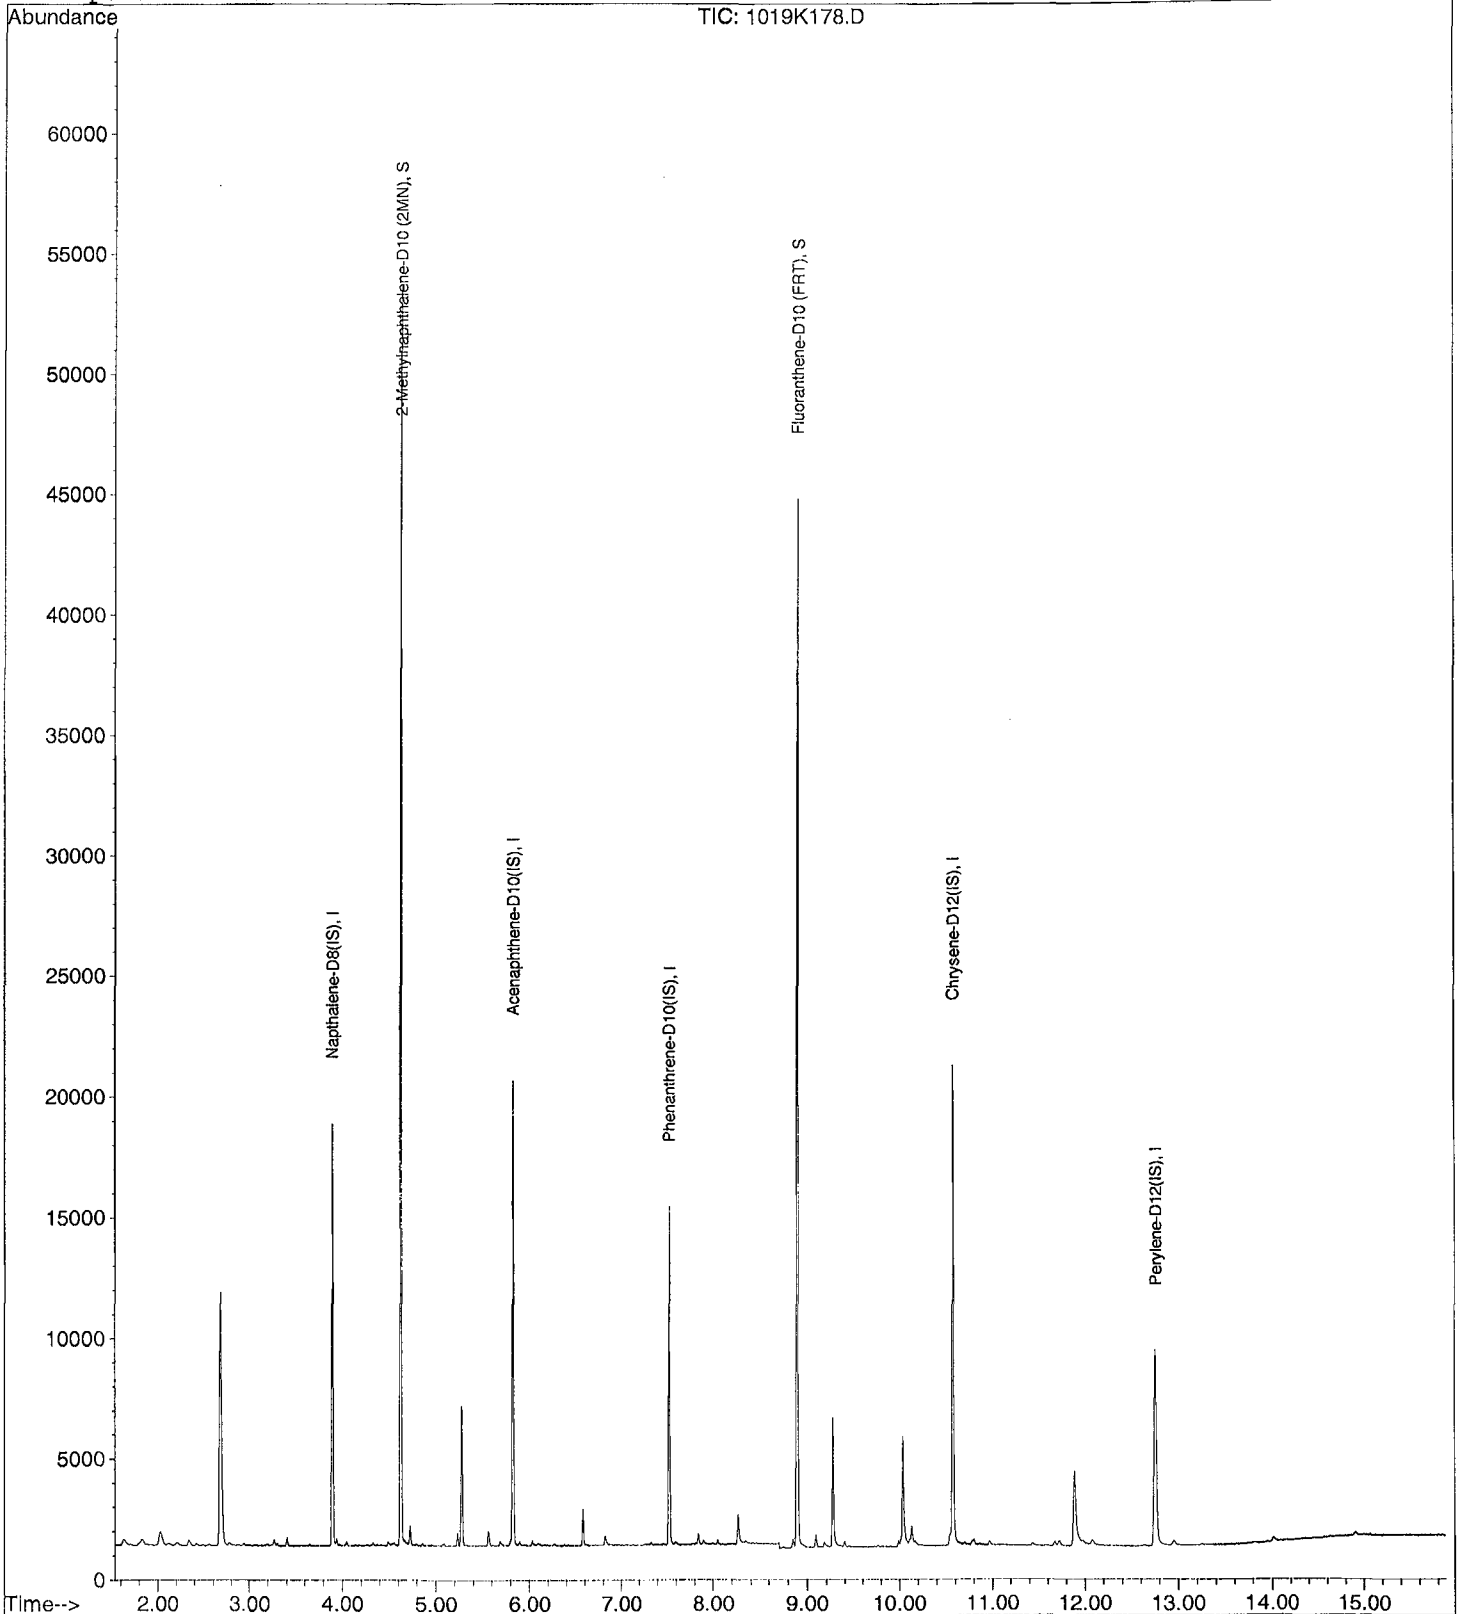

Quantitation Report (QT Reviewed)

Data File : M:\KYLO\DATA\211019\1019K172.D Vial: 22
 Acq On : 28 Oct 21 9:56 Operator: LS
 Sample : 211022A BLK 1/1000 Inst : KYLO
 Misc : Multiplr: 1.00

Quant Time: Oct 28 9:23 2021 Quant Results File: K1019.RES

Quant Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)
 Title : EPA 8270
 Last Update : Wed Oct 27 10:57:36 2021
 Response via : Initial Calibration
 DataAcq Meth : SIM_2

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Napthalene-D8 (IS)	3.89	136	12905	2.50	ppb	0.00
6) Acenaphthene-D10 (IS)	5.82	164	6299	2.50	ppb	-0.03
10) Phenanthrene-D10 (IS)	7.53	188	9803	2.50	ppb	-0.03
15) Chrysene-D12 (IS)	10.59	240	11444	2.50	ppb	-0.03
20) Perylene-D12 (IS)	12.76	264	10357	2.50	ppb	-0.07
System Monitoring Compounds						
3) 2-Methylnaphthalene-D10 (2)	4.63	152	25470	3.86	ppb	-0.03
Spiked Amount	5.000		Recovery	=	77.300%	
13) Fluoranthene-D10 (FRT)	8.90	212	31510	4.12	ppb	-0.03
Spiked Amount	5.000		Recovery	=	82.460%	

Target Compounds Qvalue

Quantitation Report


Data File : M:\KYLO\DATA\211019\1019K172.D
Acq On : 28 Oct 21 9:56
Sample : 211022A BLK 1/1000
Misc :

Vial: 22
Operator: LS
Inst : KYLO
Multiplr: 1.00

Quant Time: Oct 28 9:23 2021

Quant Results File: K1019.RES

Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)
Title : EPA 8270
Last Update : Tue Nov 09 10:14:45 2021
Response via : Initial Calibration

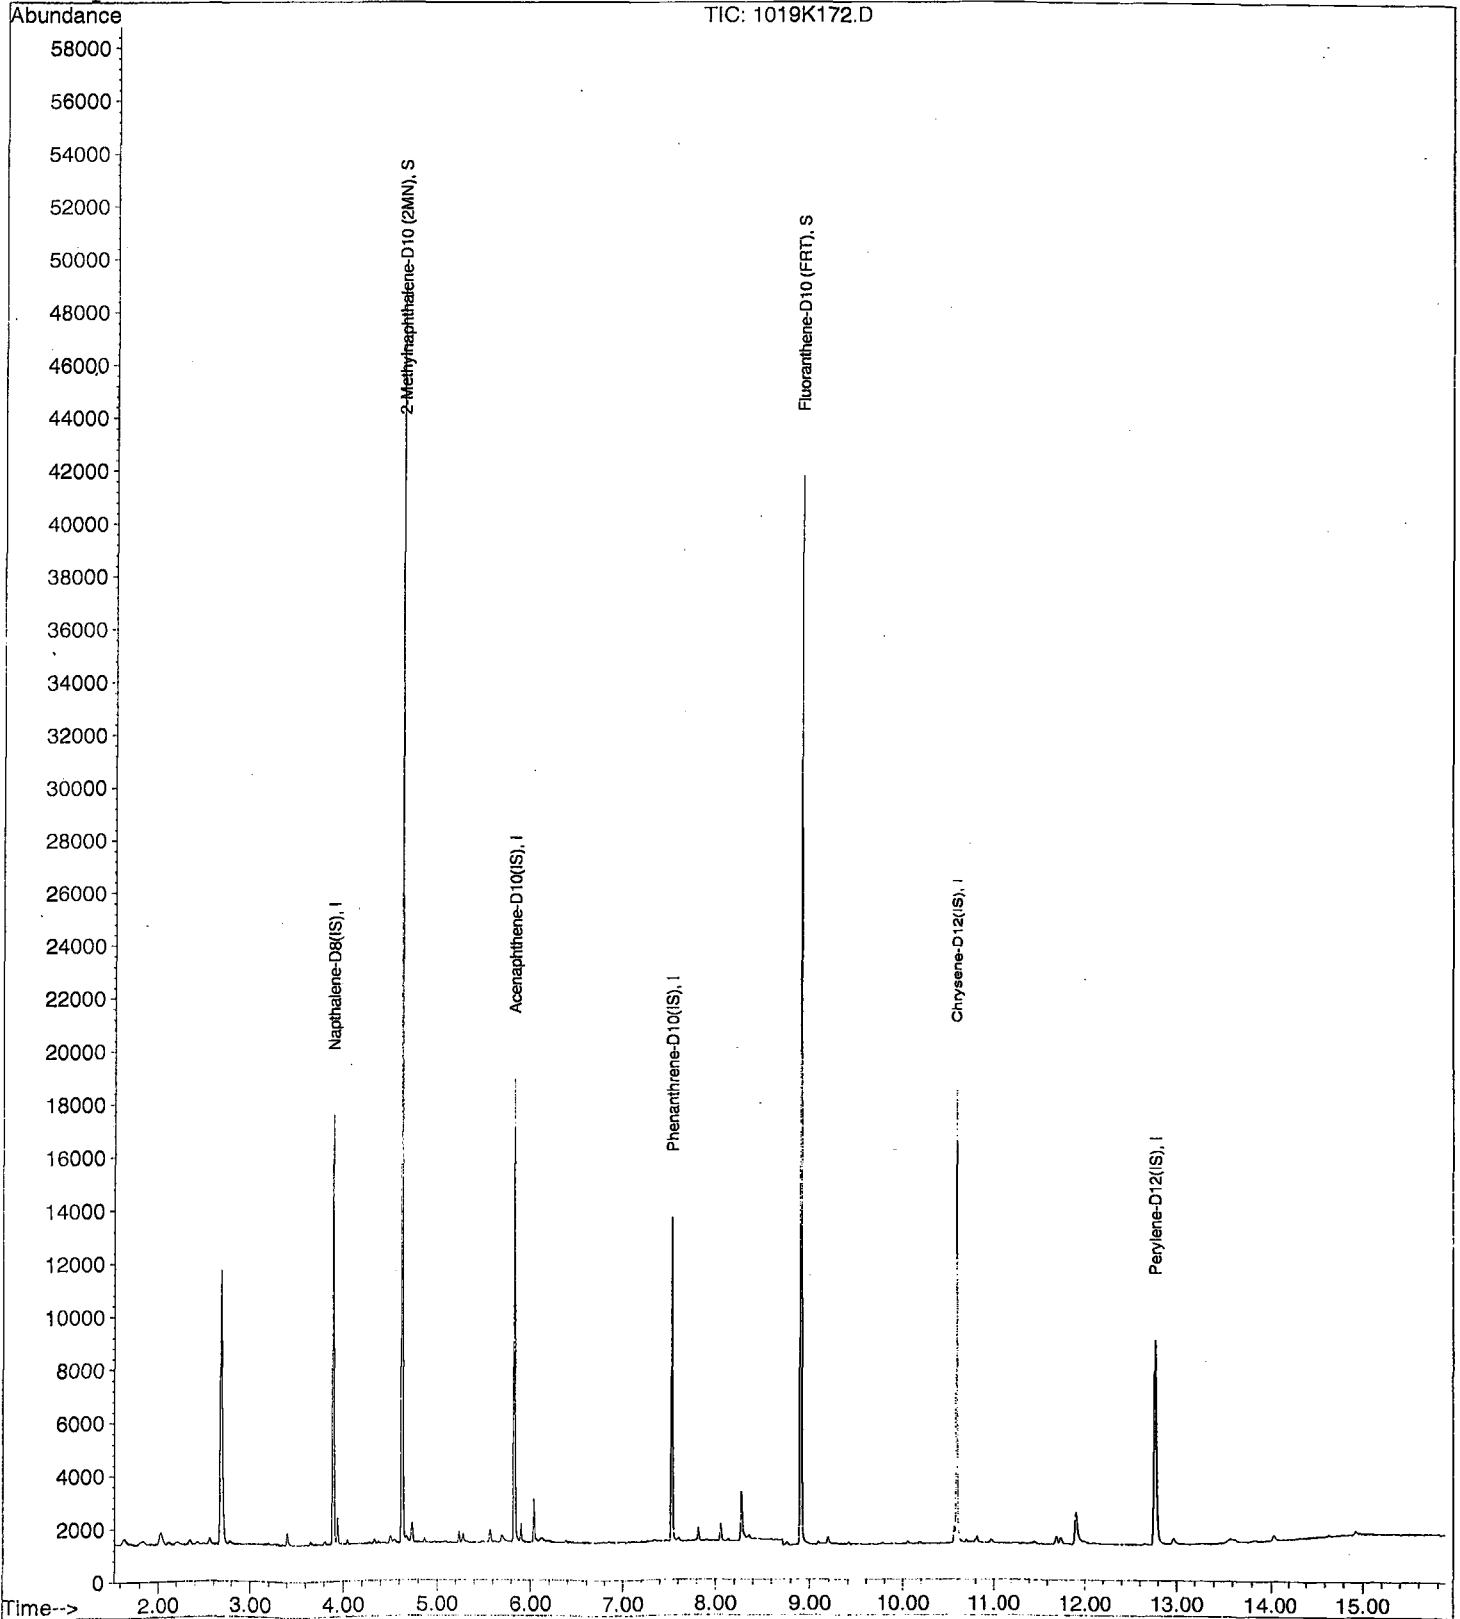

Quantitation Report (QT Reviewed)

Data File : M:\KYLO\DATA\211019\1019K173.D
 Acq On : 28 Oct 21 10:16
 Sample : 211022A LCS-1 1/1000
 Misc :

Vial: 23
 Operator: LS
 Inst : KYLO
 Multiplr: 1.00

Quant Time: Oct 28 9:56 2021

Quant Results File: K1019.RES

Quant Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)
 Title : EPA 8270
 Last Update : Wed Oct 27 10:57:36 2021
 Response via : Initial Calibration
 DataAcq Meth : SIM_2

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Napthalene-D8 (IS)	3.89	136	13479	2.50	ppb	0.00
6) Acenaphthene-D10 (IS)	5.82	164	6711	2.50	ppb	-0.03
10) Phenanthrene-D10 (IS)	7.52	188	10307	2.50	ppb	-0.03
15) Chrysene-D12 (IS)	10.57	240	12396	2.50	ppb	-0.04
20) Perylene-D12 (IS)	12.76	264	11238	2.50	ppb	-0.07
System Monitoring Compounds						
3) 2-Methylnaphthalene-D10 (2)	4.63	152	29041	4.22	ppb	-0.03
Spiked Amount	5.000		Recovery	=	84.380%	
13) Fluoranthene-D10 (FRT)	8.90	212	35459	4.41	ppb	-0.04
Spiked Amount	5.000		Recovery	=	88.260%	
Target Compounds						
2) Naphthalene	3.91	128	28856	4.12	ppb	100
4) 2-Methylnaphthalene	4.66	142	17517	4.27	ppb	99
5) 1-Methylnaphthalene	4.77	142	17506	4.23	ppb	98
7) Acenaphthylene	5.66	152	59961	4.32	ppb	99
8) Acenaphthene	5.86	154	15652	4.25	ppb	99
9) Fluorene	6.45	166	18961	4.45	ppb	100
11) Phenanthrene	7.55	178	25757	4.54	ppb	99
12) Anthracene	7.61	178	23722	4.43	ppb	99
14) Fluoranthene	8.92	202	41989	4.77	ppb	97
16) Pyrene	9.17	202	42860	4.52	ppb	97
17) Benz (a) anthracene	10.56	228	32972	4.75	ppb	100
18) Chrysene	10.61	228	33880	4.39	ppb	100
19) Indeno (1,2,3-cd). pyrene	14.32	276	24789	4.46	ppb	99
21) Benzo (b) fluoranthene	12.08	252	31501	4.98	ppb	99
22) Benzo (k) fluoranthene	12.12	252	32431	4.48	ppb	99
23) Benzo (a) pyrene	12.65	252	27927	4.63	ppb	99
24) Dibenz (a,h) anthracene	14.36	278	27258	4.57	ppb	99
25) Benzo (g,h,i) perylene	14.63	276	30037	4.63	ppb	99

Quantitation Report


Data File : M:\KYLO\DATA\211019\1019K173.D
Acq On : 28 Oct 21 10:16
Sample : 211022A LCS-1 1/1000
Misc :

Vial: 23
Operator: LS
Inst : KYLO
Multiplr: 1.00

Quant Time: Oct 28 9:56 2021

Quant Results File: K1019.RES

Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)
Title : EPA 8270
Last Update : Tue Nov 09 10:14:45 2021
Response via : Initial Calibration

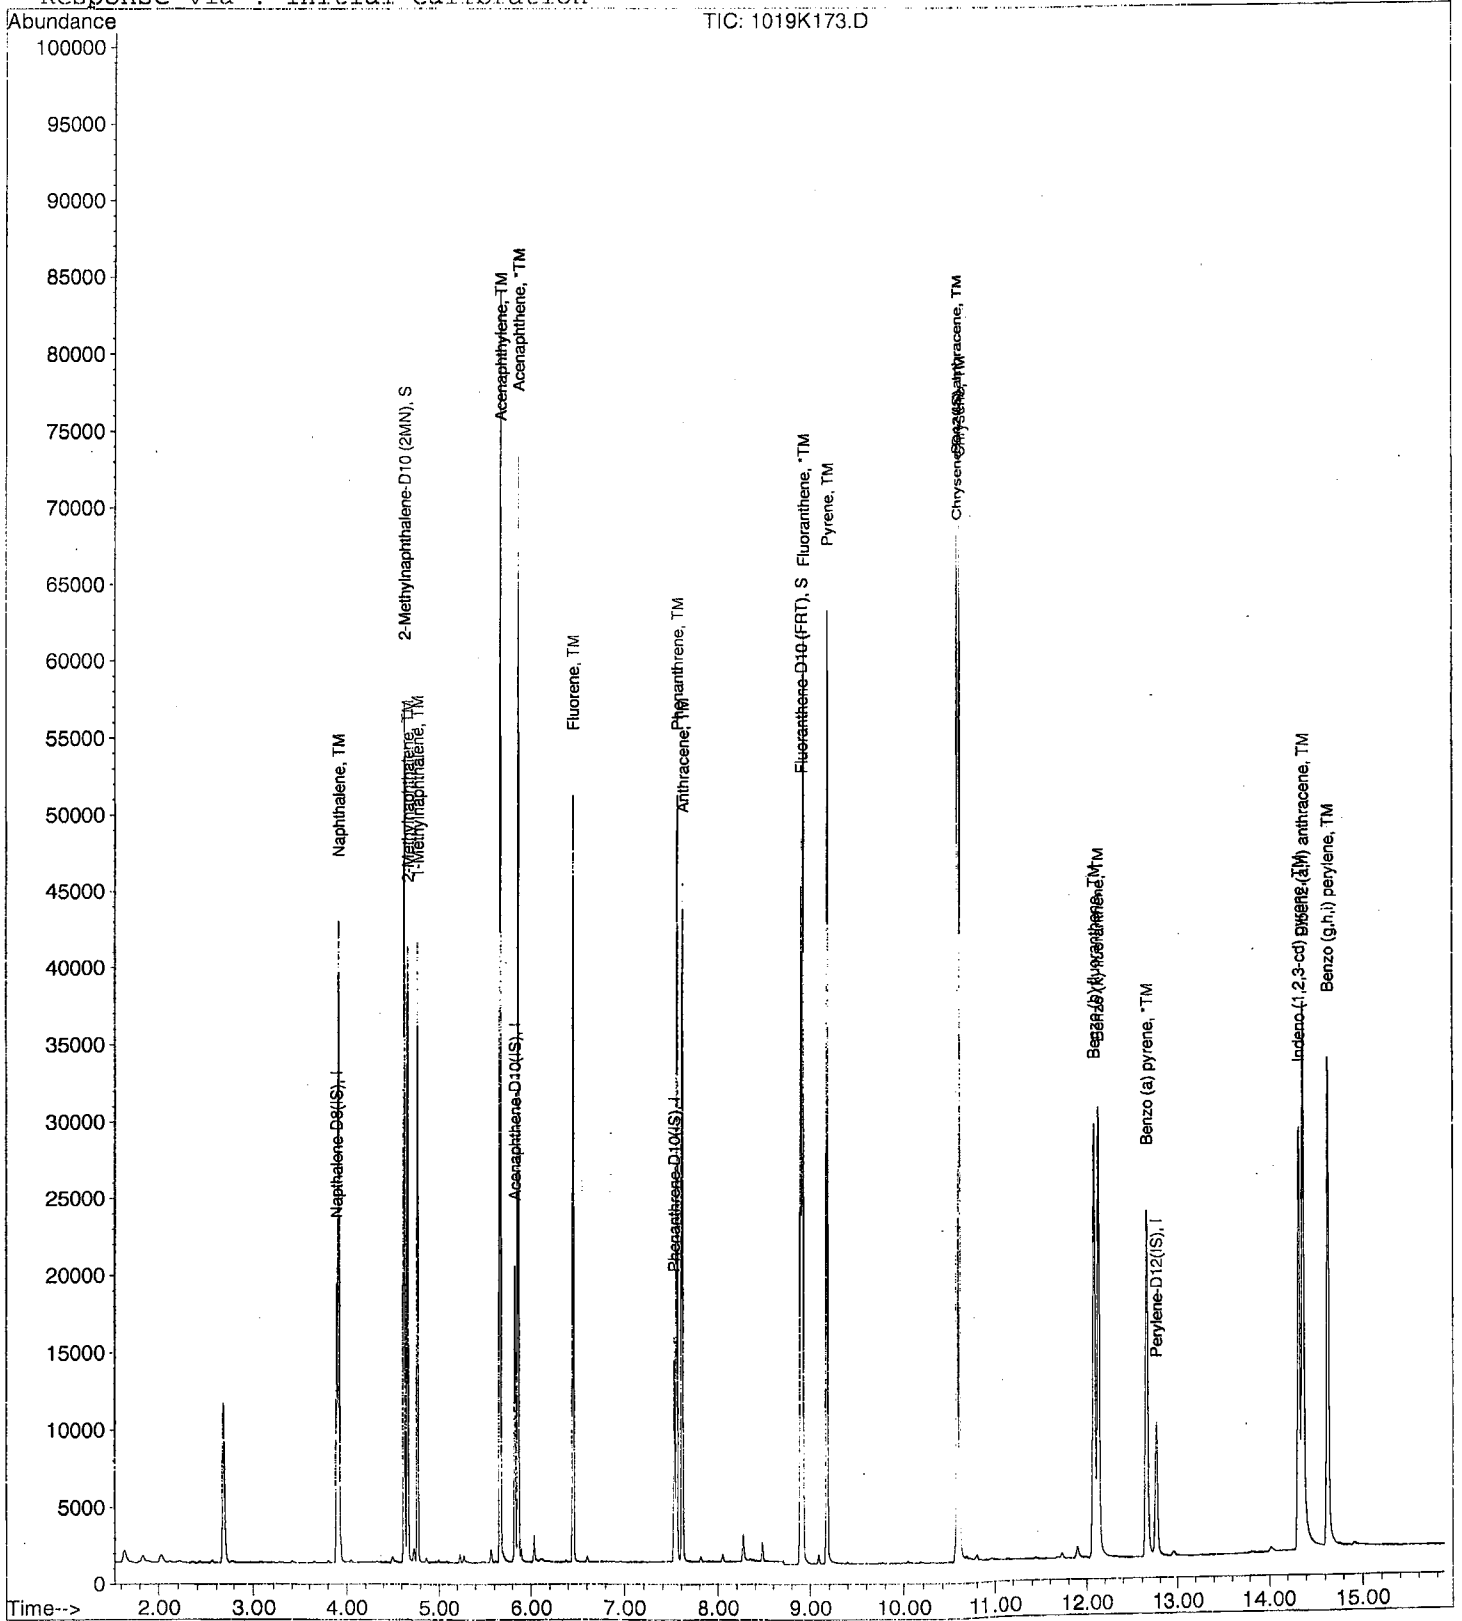

Quantitation Report (QT Reviewed)

Data File : M:\KYLO\DATA\211019\1019K174.D Vial: 24
 Acq On : 28 Oct 21 10:36 Operator: LS
 Sample : 211022A LCSD-1 1/1000 Inst : KYLO
 Misc : Multiplr: 1.00

Quant Time: Oct 28 9:56 2021 Quant Results File: K1019.RES

Quant Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)
 Title : EPA 8270
 Last Update : Wed Oct 27 10:57:36 2021
 Response via : Initial Calibration
 DataAcq Meth : SIM_2

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Napthalene-D8 (IS)	3.89	136	13301	2.50	ppb	0.00
6) Acenaphthene-D10 (IS)	5.82	164	6681	2.50	ppb	-0.03
10) Phenanthrene-D10 (IS)	7.52	188	10357	2.50	ppb	-0.03
15) Chrysene-D12 (IS)	10.57	240	12395	2.50	ppb	-0.04
20) Perylene-D12 (IS)	12.75	264	11334	2.50	ppb	-0.08
System Monitoring Compounds						
3) 2-Methylnaphthalene-D10 (2)	4.63	152	30408	4.48	ppb	-0.03
Spiked Amount	5.000		Recovery	=	89.540%	
13) Fluoranthene-D10 (FRT)	8.90	212	37223	4.61	ppb	-0.04
Spiked Amount	5.000		Recovery	=	92.200%	
Target Compounds						
2) Naphthalene	3.91	128	31490	4.56	ppb	100
4) 2-Methylnaphthalene	4.66	142	19214	4.74	ppb	98
5) 1-Methylnaphthalene	4.77	142	18958	4.64	ppb	98
7) Acenaphthylene	5.66	152	64945	4.70	ppb	100
8) Acenaphthene	5.86	154	17150	4.68	ppb	99
9) Fluorene	6.45	166	20541	4.84	ppb	99
11) Phenanthrene	7.55	178	27627	4.85	ppb	99
12) Anthracene	7.61	178	25291	4.70	ppb	99
14) Fluoranthene	8.92	202	45156	5.10	ppb	97
16) Pyrene	9.17	202	46128	4.86	ppb	97
17) Benz (a) anthracene	10.56	228	35285	5.08	ppb	100
18) Chrysene	10.61	228	36508	4.73	ppb	99
19) Indeno (1,2,3-cd) pyrene	14.31	276	26913	4.83	ppb	95
21) Benzo (b) fluoranthene	12.08	252	33019	5.17	ppb	99
22) Benzo (k) fluoranthene	12.12	252	36060	4.94	ppb	99
23) Benzo (a) pyrene	12.65	252	29936	4.92	ppb	99
24) Dibenz (a,h) anthracene	14.36	278	29371	4.89	ppb	99
25) Benzo (g,h,i) perylene	14.63	276	32214	4.92	ppb	98

Quantitation Report


Data File : M:\KYLO\DATA\211019\1019K174.D
Acq On : 28 Oct 21 10:36
Sample : 211022A LCSD-1 1/1000
Misc :

Vial: 24
Operator: LS
Inst : KYLO
Multiplr: 1.00

Quant Time: Oct 28 9:56 2021

Quant Results File: K1019.RES

Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)
Title : EPA 8270
Last Update : Tue Nov 09 10:14:45 2021
Response via : Initial Calibration


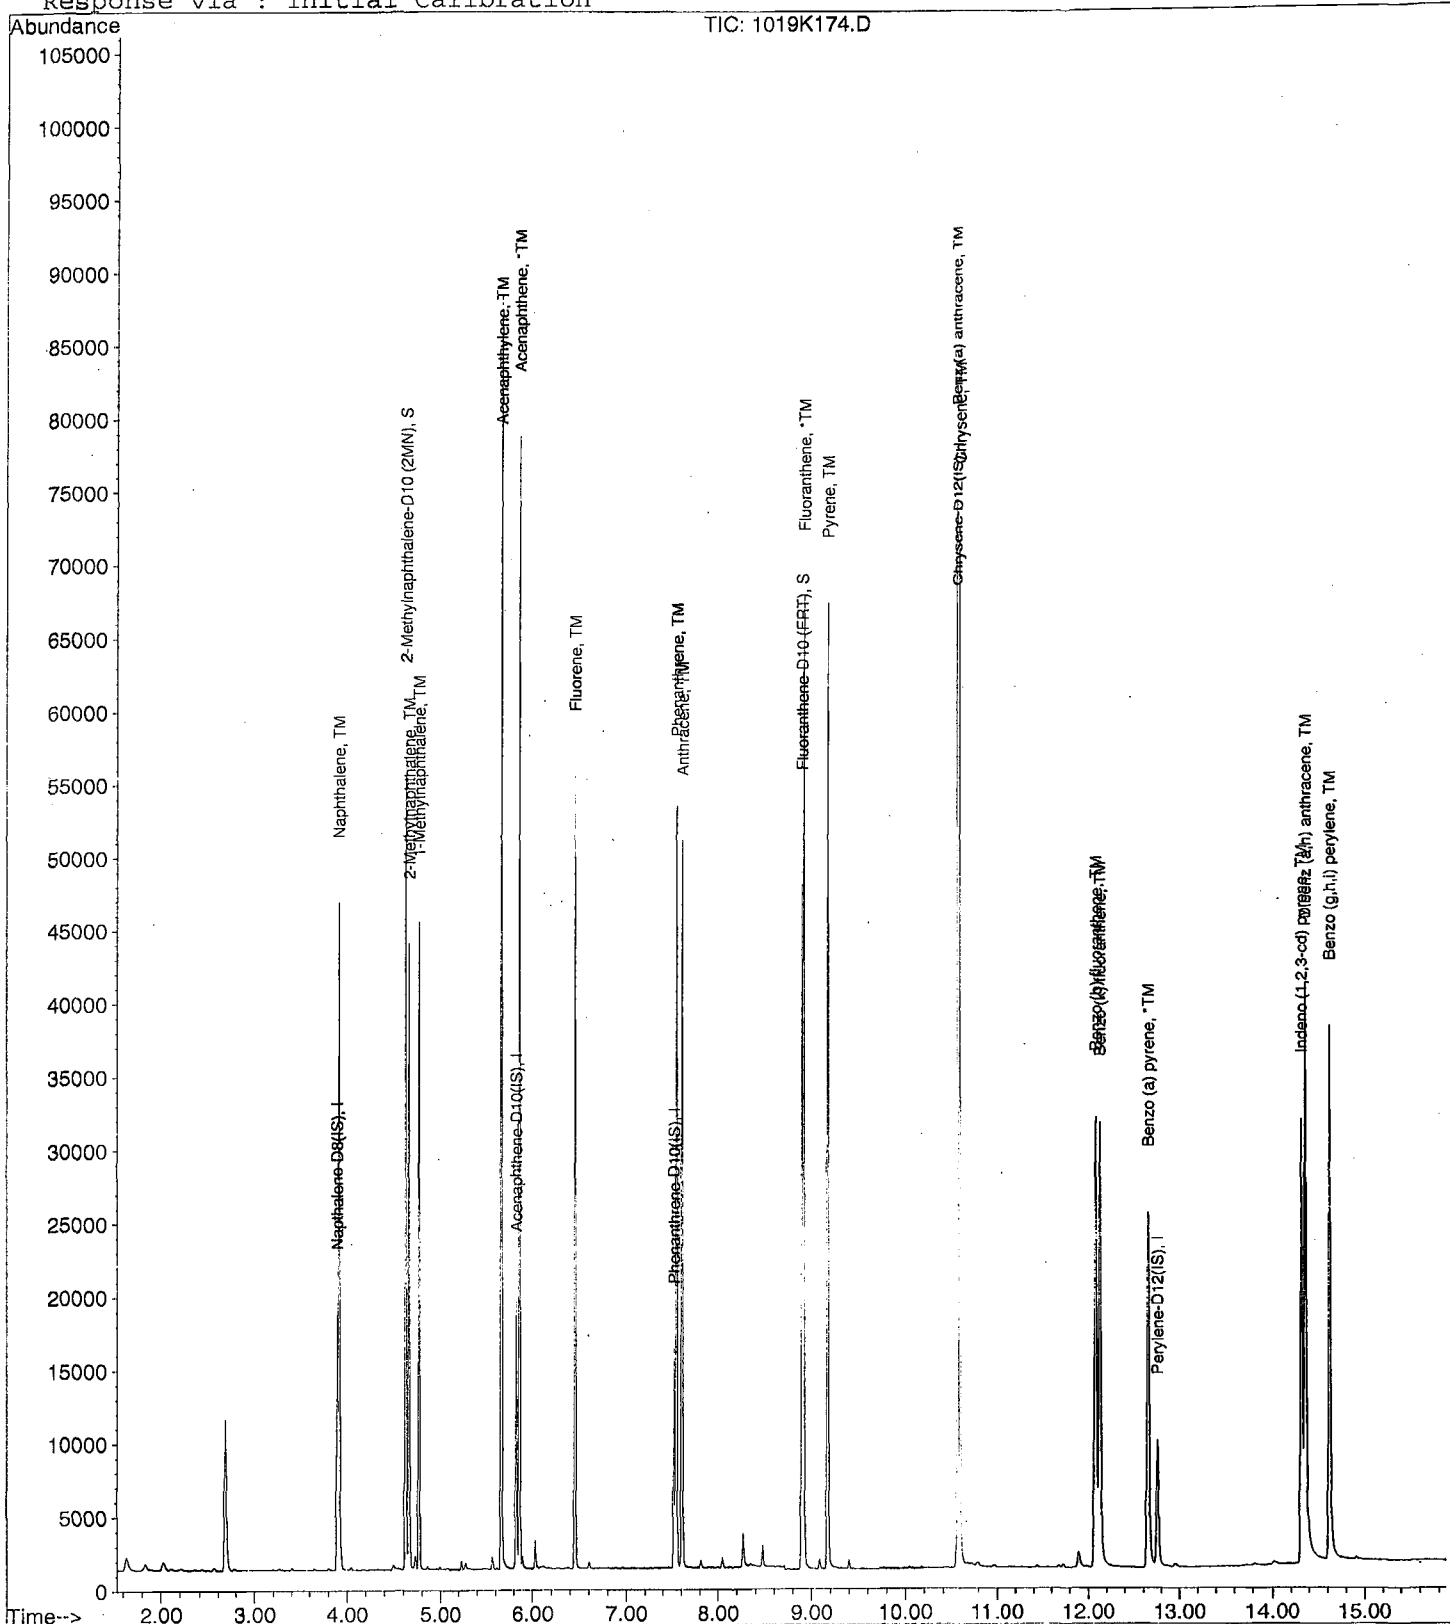


DFTPP

Data File : M:\KYLO\DATA\211019\1019K001.D
 Acq On : 19 Oct 21 13:58
 Sample : SV TUNE 7/2/21
 Misc :

Vial: 1
 Operator: LS
 Inst : KYLO
 Multiplr: 1.00

Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)
 Title : EPA 8270

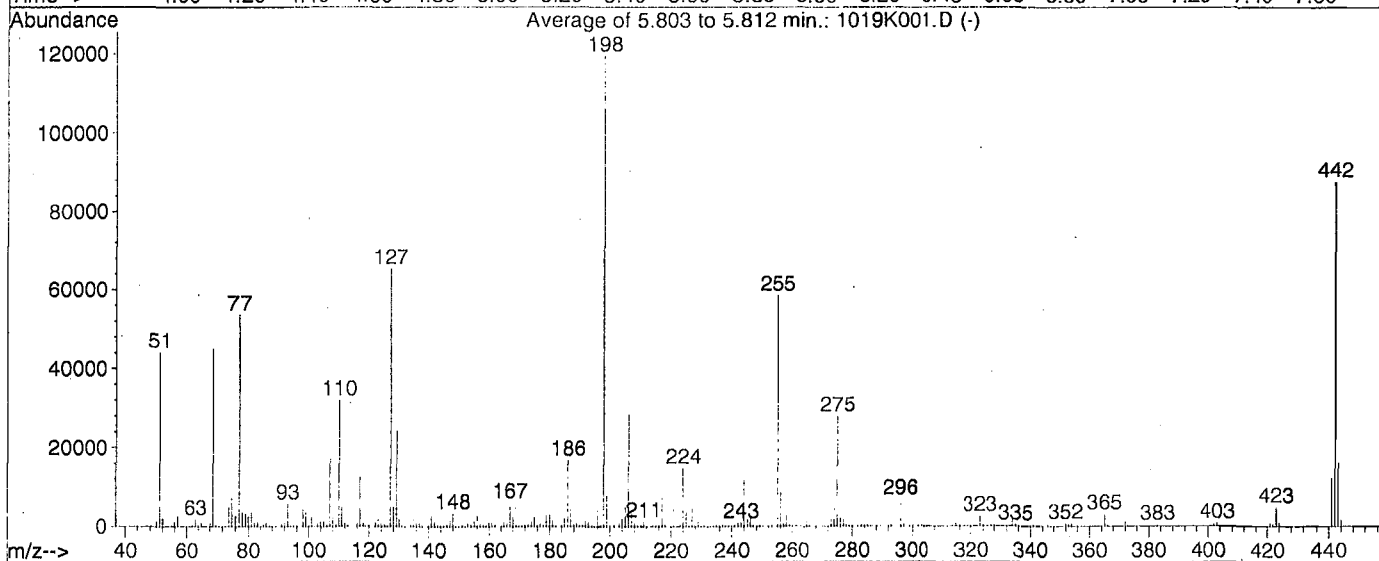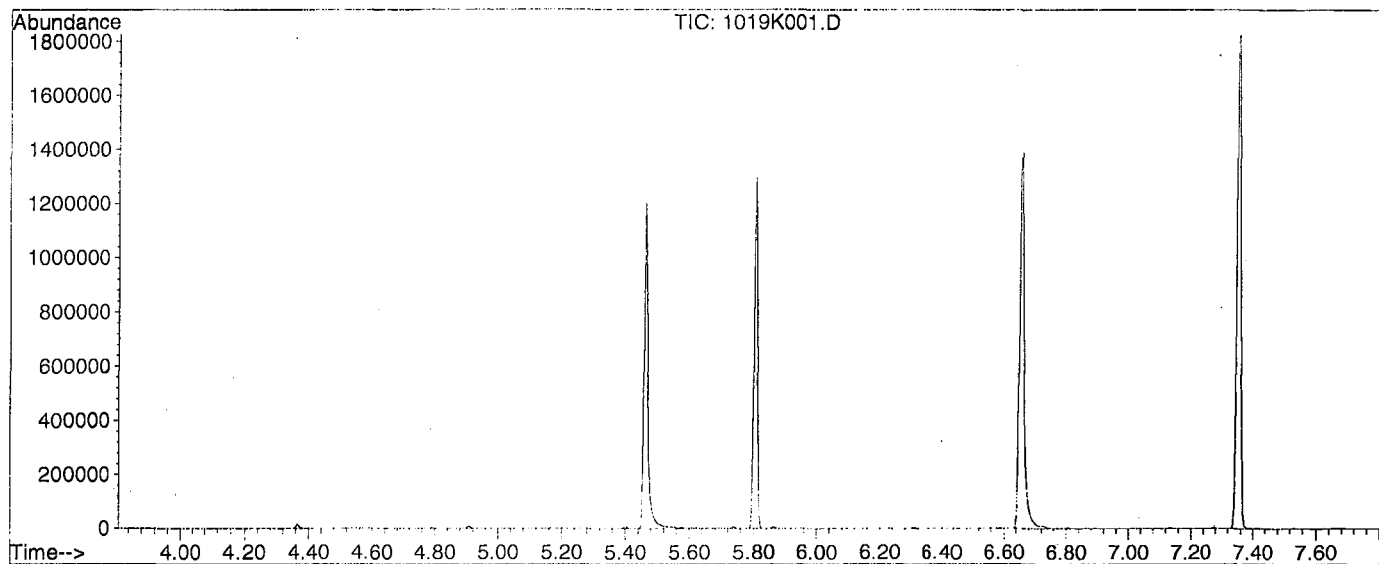

AutoFind: Scans 476, 477, 478; Background Corrected with Scan 470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	44033	PASS
68	69	0.00	2	1.7	772	PASS
70	69	0.00	2	0.4	170	PASS
127	198	10	80	54.6	65376	PASS
197	198	0.00	2	0.2	185	PASS
198	198	100	100	100.0	119640	PASS
199	198	5	9	6.5	7734	PASS
275	198	10	60	23.2	27808	PASS
365	198	1	100	2.5	3043	PASS
441	442	0.01	24	13.9	12169	PASS
442	198	50	500	73.4	87760	PASS
443	442	15	24	18.4	16149	PASS

M:\KYLO\DATA\211019\1019K001.D

Data File Name: 1019K001.D
Data File Path: M:\KYLO\DATA\211019\
Operator: LS
Date Acquired: 19 Oct 2021 13:58
Method File: K1019.M
Sample Name: SV TUNE 7/2/21
Vial Number: 1
Instrument Name: KYLO



#	Name	Ret Time	Target Response
1)	DDT	7.36	16763500
2)	DDD	7.13	0
3)	DDE	6.80	0

Breakdown 0.00

Data File : M:\KYLO\DATA\211019\1019K170.D
 Acq On : 28 Oct 21 9:06
 Sample : SV TUNE 7/2/21
 Misc :

Vial: 20
 Operator: LS
 Inst : KYLO
 Multiplr: 1.00

Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)
 Title : EPA 8270

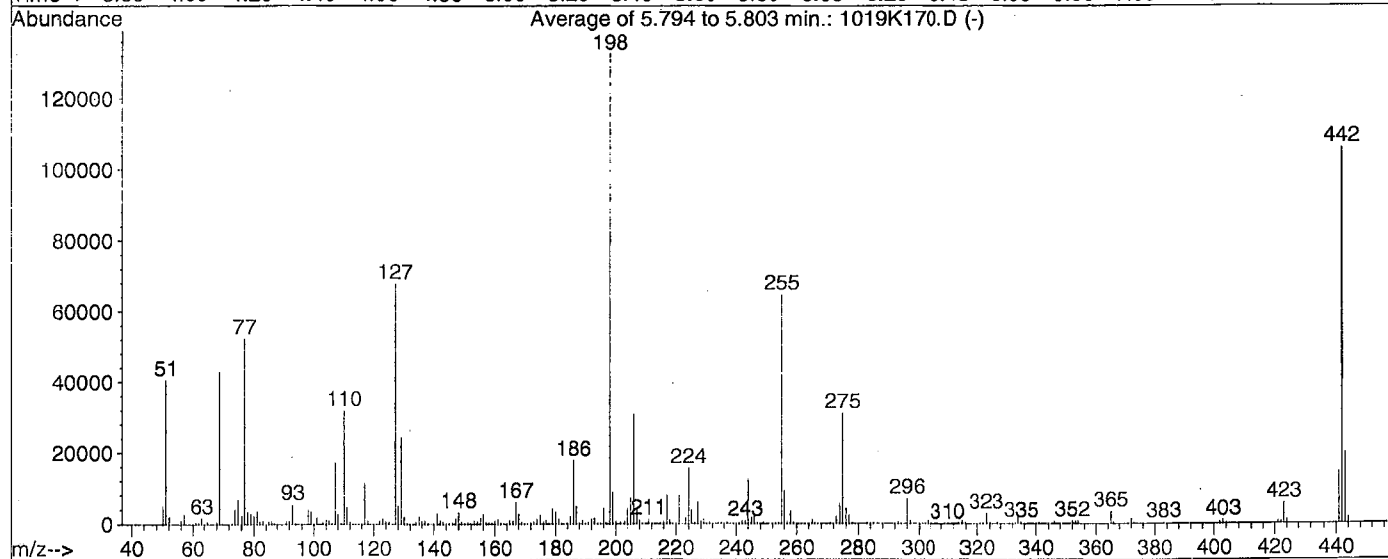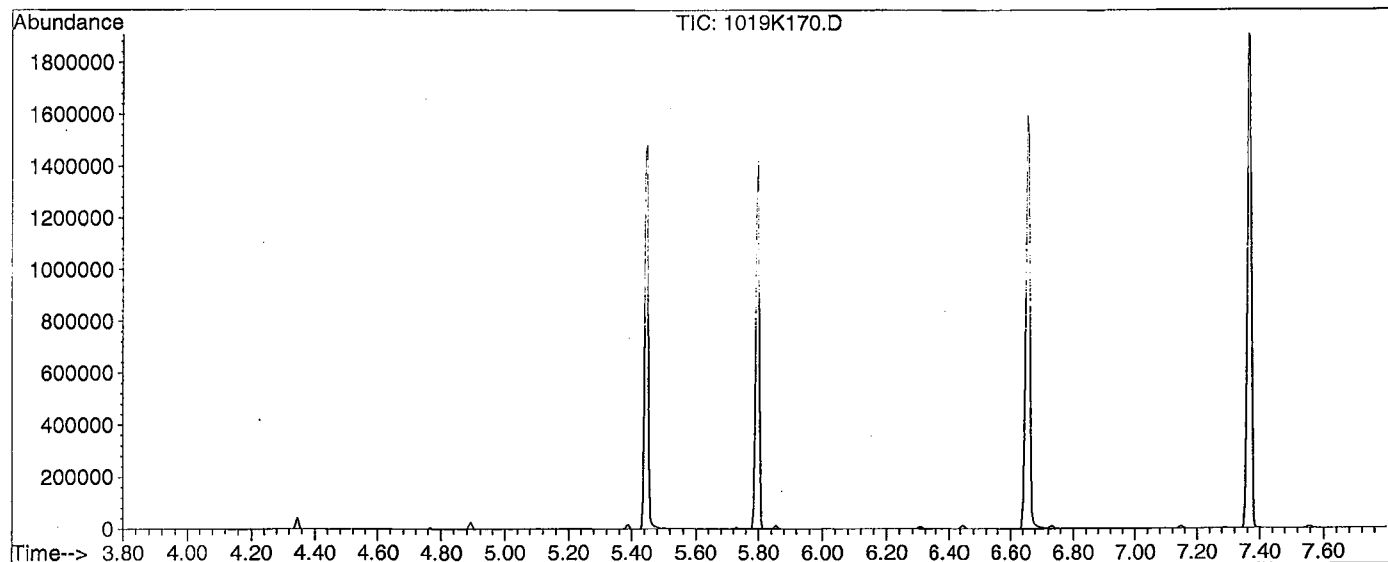

AutoFind: Scans 474, 475, 476; Background Corrected with Scan 468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.6	40600	PASS
68	69	0.00	2	1.5	635	PASS
70	69	0.00	2	0.5	211	PASS
127	198	10	80	51.2	67893	PASS
197	198	0.00	2	0.3	339	PASS
198	198	100	100	100.0	132621	PASS
199	198	5	9	6.6	8786	PASS
275	198	10	60	23.5	31197	PASS
365	198	1	100	2.5	3370	PASS
441	442	0.01	24	13.7	14506	PASS
442	198	50	500	80.0	106149	PASS
443	442	15	24	18.8	19920	PASS

M:\KYLO\DATA\211019\1019K170.D

Data File Name: 1019K170.D
Data File Path: M:\KYLO\DATA\211019\
Operator: LS
Date Acquired: 28 Oct 2021 09:06
Method File: K1019.M
Sample Name: SV TUNE 7/2/21
Vial Number: 20
Instrument Name: KYLO

#	Name	Ret Time	Target Response
1)	DDT	7.29	17317900
2)	DDD	7.07	0
3)	DDE	6.75	0

Breakdown 0.00

Name of Final Standard PAH SIM Stock (Ampule)
Prep Date 6/17/2021
Exp Date 6/17/2022

Prep'd By (Initials) LS

Initial Standard Information					Final Standard Information				
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc.(range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
Custom PAH SIM Mix	Phenova	ALO-130490	200 ug/mL	CL13121-52443	12/31/2022	1000 uL	1mL	NA	200 ug/mL

Name of Final Standard SIM Surrogate
Prep Date 6/17/2021
Exp Date 6/17/2022

Prep'd By (Initials) LS

Initial Standard Information					Final Standard Information				
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc.(range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
Sim Surrogate Deuterated	Restek	33913	2000 ug/mL	A0161454-50793	5/31/2026	1 mL	20 mL	Acetone #0246130	100 ug/mL

Name of Final Standard 8270 SIM PAH Internal Standard
Prep Date 6/17/2021
Exp Date 6/17/2022

Prep'd By (Initials) LS

Initial Standard Information					Final Standard Information				
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc.(range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
SV Internal Standard	Restek	31206	2000 ug/mL	A0162879-50593	6/30/2026	625uL	10mL	MC 60338	125 ug/mL

Name of Final Standard SIM SS Stock (Ampule second source)
Prep Date 6/17/2021
Exp Date 6/17/2022

Prep'd By LS

Initial Standard Information					Final Standard Information				
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc.(range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
Custom PAH SIM Mix	Phenova	ALO-130490	200 ug/mL	CL13117-51757	12/31/2022	1000 uL	1mL	NA	200 ug/mL

Name of Final Standard

SIM Curve

Prep'd By (Initials)

LS

Prep Date

10/13/2021

Exp Date

6/17/2022

Initial Standard Information						Final Standard Information			
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc. (range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
1.0 ug/mL SIM	APPL	1.0 ug/mL SIM	1.0 ug/mL	9/9/2021	6/17/2022	10 uL	100uL	MC 61117 90uL	0.1 ug/mL
SIM Internal Standard	APPL	SIM Internal Standard	125 ug/mL	6/17/2021	6/17/2022	2 uL	*	*	2.5ug/mL
1.0 ug/mL SIM	APPL	1.0 ug/mL SIM	1.0 ug/mL	9/9/2021	6/17/2022	20 uL	100uL	MC 61117 80uL	0.2 ug/mL
SIM Internal Standard	APPL	SIM Internal Standard	125 ug/mL	6/17/2021	6/17/2022	2 uL	*	*	2.5ug/mL
5.0 ug/mL SIM	APPL	5.0 ug/mL SIM	5.0 ug/mL	9/9/2021	6/17/2022	10 uL	100uL	MC 61117 90uL	0.5 ug/mL
SIM Internal Standard	APPL	SIM Internal Standard	125 ug/mL	6/17/2021	6/17/2022	2 uL	*	*	2.5ug/mL
5.0 ug/mL SIM	APPL	5.0 ug/mL SIM	5.0 ug/mL	9/9/2021	6/17/2022	20 uL	100uL	MC 61117 80 uL	1.0 ug/mL
SIM Internal Standard	APPL	SIM Internal Standard	125 ug/mL	6/17/2021	6/17/2022	2 uL	*	*	2.5ug/mL
SIM STOCK	APPL	SIM STOCK	200 ug/mL	6/17/2021	6/17/2022	5 uL	200uL	MC 61117 190 uL	5.0 ug/mL
SIM SURROGATE	APPL	SIM SURR	100 ug/mL	6/17/2021	6/17/2022	5 uL	*	*	2.5ug/mL
SIM Internal Standard	APPL	SIM Internal Standard	125 ug/mL	6/17/2021	6/17/2022	4 uL	*	*	2.5ug/mL
SIM STOCK	APPL	SIM STOCK	200 ug/mL	6/17/2021	6/17/2022	5 uL	100 uL	MC 61117 90 uL	10 ug/mL
SIM SURROGATE	APPL	SIM SURR	100 ug/mL	6/17/2021	6/17/2022	5 uL	*	*	5 ug/mL
SIM Internal Standard	APPL	SIM Internal Standard	125 ug/mL	6/17/2021	6/17/2022	2 uL	*	*	2.5ug/mL
SIM STOCK	APPL	SIM STOCK	200 ug/mL	6/17/2021	6/17/2022	25 uL	100uL	MC 61117 50 uL	50 ug/mL
SIM SURROGATE	APPL	SIM SURR	100 ug/mL	6/17/2021	6/17/2022	25 uL	*	*	25 ug/mL
SIM Internal Standard	APPL	SIM Internal Standard	125 ug/mL	6/17/2021	6/17/2022	2 uL	*	*	2.5ug/mL
SIM STOCK	APPL	SIM STOCK	200 ug/mL	6/17/2021	6/17/2022	50 uL	100uL	na	100 ug/mL
SIM SURROGATE	APPL	SIM SURR	100 ug/mL	6/17/2021	6/17/2022	50 uL	*	*	50 ug/mL
SIM Internal Standard	APPL	SIM Internal Standard	125 ug/mL	6/17/2021	6/17/2022	2 uL	*	*	2.5ug/mL

Name of Final Standard

8270 PAH SIM Second Source

Prep'd By (Initials)

LS

Prep Date

10/13/2021

Exp Date

6/17/2022

Initial Standard Information						Final Standard Information			
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc. (range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
PAH SIM SS Stock	Phenova	AL0-130490	200 ug/mL	6/17/2021	6/17/2022	5 uL	200uL	MC 61117 195uL	5 ug/mL
SIM Internal Standard	APPL	SIM Internal Standard	125 ug/mL	6/17/2021	6/17/2022	4 uL	*	*	2.5ug/mL

Name of Final Standard 5 SIM CCV (2x)
 Prep Date 10/19/2021
 Exp Date 6/17/2022

Prep'd By (Initials) LS

Initial Standard Information						Final Standard Information			
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc.(range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
SIM STOCK	APPL	SIM STOCK	200 ug/mL	6/17/2021	12/31/2022	5 uL	200uL	MC 61117 190 uL	5.0 ug/mL
SIM SURROGATE	APPL	SIM SURR	100 ug/mL	6/17/2021	5/31/2026	5 uL	*	*	2.5ug/mL
SIM Internal Standard	APPL	SIM Internal Standard	125 ug/mL	6/17/2021	6/30/2026	4 uL	*	*	2.5ug/mL

Name of Final Standard Semivolatfile (SV) Tuning Solution
 Prep Date 7/2/2021
 Exp Date 7/2/2022

Prep'd By (Initials) LS

Initial Standard Information						Final Standard Information			
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc.(range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
Semivolatfile GC/MS Tuning Standard	Agilent	GCM-150-1	1,000 ug/mL	6559405-51018	7/2/2022	1,000 uL	20 mL	MC #60338	50 ug/mL

Name of Final Standard SIM Spike
 Prep Date 8/5/2021
 Exp Date 5/28/2022

Prep'd By (Initials) LS

Initial Standard Information						Final Standard Information			
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc.(range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
Custom PAH Sim Mix	Phenova	AL0-130490	200 ug/mL	CL13121- 50766,50767,50771,52444,52 445	5/28/2022	5 mL	25 mL	Acetone 0246130	40 ug/mL

Name of Final Standard SIM Surrogate
 Prep Date 10/21/2021
 Exp Date 10/21/2022

Prep'd By (Initials) LS

Initial Standard Information						Final Standard Information			
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc.(range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
Sim Surrogate Deuterated	Restek	33913	2000 ug/mL	A0161454-50791,50792,50794 A0173323-52638	5/31/2027	1.5 mL	30 mL	Acetone #0246130	100 ug/mL

Organic Extraction Worksheet

Method	Continuous Liquid/Liquid SVOC 3520C	Extraction Set	211021A	Extraction Method	LIQ003	Units	mL
Spiked ID 1	Sim Spike 8-5-21 5-28-22	Surrogate ID 1	SIM Surrogate 10-21-21 10-21-22				
Spiked ID 2		Surrogate ID 2					
Spiked ID 3		Surrogate ID 3					
Spiked ID 4		Surrogate ID 4					
Spiked ID 5		Surrogate ID 5					
Spiked ID 6		Sufficient Vol for Matrix QC:		NO			
Spiked ID 7		Ext. Start Time:		10/21/21 9:43			
Spiked ID 8		Ext. End Time:		10/22/21 7:12			
GC Requires Extract By:							
pH1	14	10/21/21 8:53	Water Bath Temp 1 °C	75/74.5 E-WB5 °			
pH2	14	10/21/21 16:30	Water Bath Temp 2 °C				
pH3	14	10/22/21 9:20	Water Bath Temp 3 °C				

Spiked By: SR

Date 10/22/2021

Witnessed By: CG

Date 10/22/2021

Sample	Sample Container	Spike Amount	Spike ID	Surrogate Amount	Surrogate ID	Extract Amount	Final Volume	pH	Extract Date/Time	Comments
1 211021A Blk				0.050	1	1000	1	14	10/22/21 8:47	
					equip	E-HP3 E-WB5				
2 211021A LCS-1		0.125	1	0.050	1	1000	1	14	10/22/21 8:47	
					equip	E-HP4 E-WB5				
3 211021A LCSD-1		0.125	1	0.050	1	1000	1	14	10/22/21 8:47	
					equip	E-HP6 E-WB5				
4 BA43555	BA43555W08			0.050	1	1000	1	14	10/22/21 7:57	97901
					equip	E-HP8 E-WB5				
5 BA43832	BA43832W07			0.050	1	1000	1	14	10/22/21 16:20	97924
					equip	E-HP7 E-WB5				
6 BA43833	BA43833W05			0.050	1	1000	1	14	10/22/21 16:20	97924
					equip	E-HP9 E-WB5				
7 BA43837	BA43837W07			0.050	1	1000	1	14	10/22/21 16:20	97923
					equip	E-HP10 E-WB5				
8 BA43840	BA43840W07			0.050	1	1000	1	14	10/22/21 7:57	97918
					equip	E-HP17 E-WB5				

Solvent and Lot#	
PH Strips	HC15596
Dichloromethane (DCM)	61117
10N NaOH (10mLs)	10-18-21
Filter Paper	400196
Na2SO4	2021071206

Extraction COC Transfer	
Extraction lab employee Initials	KY
GC analyst's initials	CW
Date	10-26-21
Time	10:09
Refrigerator	GC_C

Technician's Initials	
Scanned By	SR
Sample Preparation	SR
Extraction	SR
Concentration	AGM
Modified	11/9/2021 9:44:07 AM

Reviewed By: KY

Date 10/27/2021

Injection Log

Directory: M:\KYLO\DATA\211019\

Vial	FileName	Multiplier	SampleName	Misc Info	Injected
1	1019K001.D	1	SV TUNE 7/2/21		19 Oct 21 13:58
2	1019K002.D	1	0.1 ug/ml 10/13/21		19 Oct 21 14:09
3	1019K003.D	1	0.2 ug/ml 10/13/21		19 Oct 21 14:29
4	1019K004.D	1	0.5 ug/ml 10/13/21		19 Oct 21 14:49
5	1019K005.D	1	1 ug/ml 10/13/21		19 Oct 21 15:09
6	1019K006.D	1	5 ug/ml 10/13/21		19 Oct 21 15:29
7	1019K007.D	1	10 ug/ml 10/13/21		19 Oct 21 15:49
8	1019K008.D	1	50 ug/ml 10/13/21		19 Oct 21 16:09
9	1019K009.D	1	100 ug/ml 10/13/21		19 Oct 21 16:29
10	1019K010.D	1	SS ug/ml 10/13/21		19 Oct 21 16:49
20	1019K170.D	1	SV TUNE 7/2/21		28 Oct 21 9:06
21	1019K171.D	1	5 ug/ml 10/19/21 (1)		28 Oct 21 9:18
22	1019K172.D	1	211021A BLK 1/1000		28 Oct 21 9:56
23	1019K173.D	1	211021A LCS-1 1/1000		28 Oct 21 10:16
24	1019K174.D	1	211021A LCSD-1 1/1000		28 Oct 21 10:36
28	1019K178.D	1	BA43837W07 1/1000		28 Oct 21 11:55
55	1019K205.D	1	5 ug/ml 10/13/21 (2)		28 Oct 21 20:55

ORGANICS
Calibration Data

VOLATILE ORGANIC ANALYSIS BY
EPA METHOD 8260B

Form 6
Initial Calibration

Lab Name: APPL, Inc.

SDG No:

Case No:

Initial Cal. Date: 10/15/2021

Matrix: Water

Instrument: Max

Initials: _____

1015M12.D 1015M13.D 1015M14.D 1015M15.D 1015M16.D 1015M17.D 1015M18.D 1015M19.D 1015M20.D

	Compound	1	2	3	4	5	6	7	8	9		Avg	%RSD	Type	r^2	Q	MRF
1	I Fluorobenzene (IS)																
2	TM Chlorotrifluoroethene													TM			
3	TM Dichlorodifluoromethane		0.1508	0.1611	0.1414	0.1748	0.1296	0.1371	0.1510	0.1516		0.15	9.4	TM			
4	TM Freon 114	0.0629	0.0771	0.0867	0.0903	0.0897	0.0706	0.0918	0.0908	0.0949		0.08	13	TM			
5	TM** Chloromethane		0.0816	0.1036	0.0852	0.0940	0.0885	0.0795	0.0895	0.0924		0.09	8.6	TM**			
6	TM* Vinyl chloride	0.1225	0.1206	0.0979	0.1015	0.1123	0.1098	0.1056	0.1118	0.1091		0.11	7.3	TM*			
7	TM 2-Chloro-1,1,1-trifluoroethane													TM			
8	TM Bromomethane	0.1252	0.0995	0.0992	0.0848	0.0948	0.0853	0.0794	0.0814	0.0879		0.09	15	TM			
9	TML Chloroethane	0.0933	0.0961	0.1579	0.0552	0.0706	0.0745	0.0641	0.0666	0.0815		0.08	36	TM	0.994		
10	TM Dichlorofluoromethane	0.2569	0.3121	0.2592	0.2176	0.2203	0.2414	0.2187	0.2235	0.2246		0.24	13	TM			
11	TM Trichlorofluoromethane	0.2324	0.3029	0.2888	0.3134	0.2973	0.2882	0.2855	0.2975	0.2941		0.29	7.9	TM			
12	TM 2,2-Dichloro-1,1,1-trifluoroethane													TM			
13	TMQ Acrolein	0.0166	0.0144	0.0135	0.0153	0.0136	0.0142	0.0135	0.0145	0.0144		0.01	7.0	TM	0.997		
14	TM Acetone	0.0398	0.0304	0.0345	0.0331	0.0310	0.0319	0.0307	0.0309	0.0310		0.03	9.3	TM			
15	TM Freon-113	0.1116	0.1300	0.1296	0.1218	0.1150	0.1068	0.1175	0.1124	0.1135		0.12	6.9	TM			
16	TM Acetonitrile	0.0101	0.0070	0.0074	0.0070	0.0076	0.0073	0.0076	0.0080	0.0077		0.01	12	TM			
17	TML 2-propanol													TM			
18	TM 1,2-Dichlorotrifluoroethane	0.2569	0.3121	0.2592	0.2176	0.2203	0.2414	0.2187	0.2235	0.2247		0.24	13	TM			
19	TM* 1,1-DCE	0.1787	0.1830	0.1897	0.1807	0.1708	0.1678	0.1697	0.1653	0.1699		0.18	4.7	TM*			
20	TMQ t-Butanol	0.0115	0.0086	0.0097	0.0102	0.0110	0.0102	0.0098				0.01	9.2	TM	0.995		
21	TMQ Methyl Acetate		0.0500	0.0481	0.0566	0.0491	0.0547	0.0536	0.0554	0.0547		0.05	6.1	TM	1.000		
22	TML Iodomethane	0.1065	0.1250	0.0882	0.0717	0.0979	0.1158	0.1130	0.1296	0.1388		0.11	19	TM	0.998		
23	TML Acrylonitrile	0.0088	0.0055	0.0298	0.0239	0.0337	0.0321	0.0316	0.0309	0.0304		0.03	42	TM	1.000		
24	TM 2-Methylpentane													TM			
25	TM Methylene chloride	0.1502	0.1032	0.1123	0.1093	0.1063	0.1155	0.1083	0.1086	0.1035		0.11	13	TM			
26	TM Carbon disulfide	0.1567	0.1530	0.1390	0.1605	0.1324	0.1389	0.1392	0.1362	0.1258		0.14	8.2	TM			
27	TM Methyl t-butyl ether (MtBE)	0.4054	0.3871	0.3993	0.3508	0.3716	0.3784	0.3615	0.3797	0.3589		0.38	4.9	TM			
28	TM Trans-1,2-DCE		0.1591	0.1103	0.1150	0.1200	0.1175	0.1222	0.1143	0.1180		0.12	13	TM			
29	TML 3-Methylpentane	0.0803	0.0784	0.0715	0.0806	0.0660	0.0664	0.0682	0.0593	0.0607		0.07	12	TM	0.999		
30	TM Hexane													TM			
31	TM Diisopropyl Ether	0.1713	0.2278	0.2501	0.2487	0.2546	0.2465	0.2359	0.2412	0.2396		0.24	11	TM			
32	TM** 1,1-DCA	0.1334	0.1964	0.2073	0.1858	0.1835	0.1860	0.1867	0.1843	0.1844		0.18	11	TM**			
33	TM Vinyl Acetate													TM			
34	TM Ethyl tert Butyl Ether	0.2869	0.3155	0.2850	0.3007	0.3100	0.3054	0.3017	0.3165	0.2971		0.30	3.7	TM			
35	TML Methylcyclopentane	0.0042	0.0425	0.0170	0.0155	0.0146	0.0129	0.0124	0.0132	0.0113		0.02	66	TM	0.996		

VOLATILE ORGANIC ANALYSIS BY
EPA METHOD 8260B

Form 6
Initial Calibration

Lab Name: APPL, Inc.
Case No: _____
Matrix: Water

SDG No: _____
Initial Cal. Date: 10/15/2021
Instrument: Max

Initials: _____

		Compound	1	2	3	4	5	6	7	8	9		Avg	%RSD	Type		Q	MRF
36	TM	MEK (2-Butanone)	0.0332	0.0326	0.0363	0.0351	0.0325	0.0357	0.0324	0.0342	0.0346		0.03	4.3	TM			
37	TM	Cis-1,2-DCE	0.1508	0.1567	0.1446	0.1113	0.1316	0.1360	0.1266	0.1312	0.1278		0.14	10	TM			
38	TM	2,2-Dichloropropane	0.2829	0.2366	0.2197	0.2193	0.2309	0.2454	0.2308	0.2242	0.2240		0.23	8.5	TM			
39	TM*	Chloroform	0.1554	0.2020	0.2501	0.2382	0.2569	0.2726	0.2578	0.2540	0.2523		0.24	15	TM*			
40	TML	Bromochloromethane	0.1040	0.0920	0.0931	0.1176	0.1094	0.1056	0.1049	0.1084	0.1009		0.10	7.7	TM	0.999		
41	S	Dibromofluoromethane(S)	0.3580	0.3340	0.3038	0.2941	0.3047	0.3136	0.2987	0.3015	0.2862		0.31	7.2	S			
42	TM	1,1,1-TCA	0.2636	0.2422	0.2707	0.2885	0.2921	0.2898	0.2963	0.2887	0.2800		0.28	6.3	TM			
43	TM	Cyclohexane	0.0786	0.0832	0.0908	0.0807	0.0825	0.0701	0.0773	0.0765	0.0788		0.08	7.0	TM			
44	TM	1,1-Dichloropropene	0.1321	0.1579	0.1511	0.1468	0.1674	0.1534	0.1551	0.1496	0.1495		0.15	6.2	TM			
45	TM	2,2,4-Trimethylpentane	0.2393	0.1672	0.2119	0.2264	0.1839	0.1678	0.1830	0.1923	0.1956		0.20	13	TM			
46	S	1,2-DCA-D4(S)	0.2537	0.2270	0.2111	0.2053	0.2170	0.2102	0.2102	0.2107	0.2039		0.22	7.2	S			
47	TM	Carbon Tetrachloride	0.2703	0.2346	0.2668	0.2614	0.2739	0.2671	0.2581	0.2643	0.2660		0.26	4.4	TM			
48	TM	Tert Amyl Methyl Ether	0.2852	0.3313	0.2672	0.2865	0.3043	0.3119	0.2953	0.3074	0.2915		0.30	6.2	TM			
49	TM	1,2-DCA	0.2196	0.2210	0.2380	0.2461	0.2367	0.2417	0.2309	0.2437	0.2374		0.24	4.0	TM			
50	TM	Benzene	0.4803	0.4517	0.4397	0.4236	0.4345	0.4448	0.4245	0.4267	0.4199		0.44	4.3	TM			
51	TM	TCE	0.1271	0.1743	0.1565	0.1358	0.1245	0.1448	0.1323	0.1347	0.1332		0.14	11	TM			
52	TM	2-Pentanone	0.0582	0.0562	0.0561	0.0572	0.0561	0.0576	0.0555	0.0577	0.0580		0.06	1.8	TM			
53	TM*L	1,2-Dichloropropane	0.0482	0.0546	0.0514	0.0360	0.0419	0.0501	0.0484	0.0514	0.0467		0.05	12	TM*	0.998		
54	TM	Bromodichloromethane	0.1483	0.2146	0.1662	0.2030	0.2205	0.2025	0.2006	0.2104	0.2051		0.20	12	TM			
55	TML	Methyl Cyclohexane	0.1984	0.1391	0.1440	0.1602	0.1519	0.1358	0.1512	0.1540	0.1531		0.15	12	TM	1.000		
56	TM	Dibromomethane	0.0944	0.0820	0.1045	0.0868	0.0845	0.0850	0.0766	0.0795	0.0773		0.09	10	TM			
57	TM	MIBK (methyl isobutyl ketone)	0.0770	0.0658	0.0724	0.0771	0.0701	0.0753	0.0704	0.0737	0.0738		0.07	5.0	TM			
58	TML	1-Bromo-2-chloroethane	0.0302	0.0087	0.0167	0.0232	0.0320	0.0269	0.0274	0.0281	0.0275		0.02	30	TM	1.000		
59	TM	2-Chloroethyl vinyl ether													TM			
60	TM	Cis-1,3-Dichloropropene	0.1208	0.1719	0.1709	0.1894	0.1907	0.1839	0.1841	0.1860	0.1894		0.18	13	TM			
61	TM*	Toluene	0.5522	0.4801	0.4779	0.4772	0.5146	0.5462	0.5004	0.5063	0.5080		0.51	5.5	TM*			
62	TM	Trans-1,3-Dichloropropene	0.1393	0.1391	0.1685	0.1795	0.1887	0.1861	0.1833	0.1944	0.1948		0.17	12	TM			
63	TM	1,1,2-TCA	0.0935	0.0961	0.0637	0.0759	0.0732	0.0810	0.0731	0.0753	0.0756		0.08	13	TM			
64	TM	2-Hexanone	0.0466	0.0396	0.0499	0.0508	0.0466	0.0527	0.0507	0.0528	0.0538		0.05	9.0	TM			
65	I	Chlorobenzene-D5 (IS)																
66	S	Toluene-D8(S)	1.339	1.273	1.107	1.107	1.129	1.132	1.110	1.106	1.038		1.1	8.2	S			
67	TM	1,2-EDB	0.1119	0.1589	0.1216	0.1371	0.1335	0.1292	0.1341	0.1299	0.1309		0.13	9.6	TM			
68	TML	Tetrachloroethene	0.6091	0.3484	0.2276	0.1756	0.1358	0.1173	0.1351	0.1232	0.1143		0.22	74	TM	0.999		
69	TM	1-Chlorohexane	0.1152	0.0891	0.1082	0.0965	0.1019	0.0897	0.0993	0.0952	0.0980		0.10	8.4	TM			
70	TM	1,1,1,2-Tetrachloroethane	0.1391	0.1828	0.1648	0.1859	0.2121	0.2018	0.1949	0.1960	0.1965		0.19	12	TM			

VOLATILE ORGANIC ANALYSIS BY
EPA METHOD 8260B

Form 6
Initial Calibration

Lab Name: APPL, Inc.
Case No: _____
Matrix: Water

SDG No: _____
Initial Cal. Date: 10/15/2021
Instrument: Max

Initials: _____

	Compound	1	2	3	4	5	6	7	8	9		Avg	%RSD	Type	Q	MRF
71	TM	m&p-Xylene	0.2844	0.2517	0.2669	0.2707	0.2937	0.2972	0.2994	0.2919	0.2876	0.28	5.7	TM		
72	TM	o-Xylene	0.3290	0.3153	0.3138	0.2563	0.2863	0.2930	0.2871	0.2939	0.2927	0.30	7.1	TM		
73	TM	Styrene	0.4104	0.4286	0.3830	0.4298	0.4621	0.4757	0.4696	0.4735	0.4835	0.45	7.8	TM		
74	S	4-Bromofluorobenzene(S)	0.5305	0.4709	0.4295	0.4339	0.4550	0.4619	0.4657	0.4698	0.4596	0.46	6.2	S		
75	TM	1,3-Dichloropropane	0.2500	0.1841	0.1902	0.1782	0.1994	0.1925	0.1833	0.1867	0.1812	0.19	11	TM		
76	TM	Dibromochloromethane	0.2041	0.1894	0.1919	0.1859	0.1928	0.1923	0.1967	0.1988	0.1947	0.19	2.8	TM		
77	TM**	Chlorobenzene	0.4530	0.4058	0.3834	0.4602	0.4488	0.4441	0.4397	0.4331	0.4323	0.43	5.6	TM**		
78	TM*	Ethylbenzene	0.8163	0.6181	0.6491	0.6508	0.7106	0.6823	0.6773	0.6899	0.6792	0.69	8.1	TM*		
79	TM**	Bromoform	0.1795	0.1248	0.1586	0.1638	0.1562	0.1606	0.1638	0.1699	0.1727	0.16	9.6	TM**		
80	I	1,4-Dichlorobenzene-D (IS)														
81	TM	Isopropylbenzene	1.406	1.232	1.129	1.052	1.159	1.126	1.148	1.104	1.137	1.2	8.7	TM		
82	TM**	1,1,2,2-Tetrachloroethane		0.2460	0.2121	0.2073	0.1907	0.1939	0.1838	0.1825	0.1841	0.20	11	TM**		
83	TM	1,2,3-Trichloropropane		0.1099	0.0947	0.1052	0.1046	0.0956	0.0992	0.0943	0.0968	0.10	5.8	TM		
84	TML	t-1,4-Dichloro-2-Butene	0.1357	0.0279	0.0748	0.0564	0.0450	0.0484	0.0489	0.0515	0.0523	0.06	51	TM	1.000	
85	TM	Bromobenzene	0.4062	0.4088	0.3460	0.4046	0.3788	0.3610	0.3870	0.3662	0.3760	0.38	5.8	TM		
86	TM	n-Propylbenzene	1.201	1.175	1.139	1.072	1.136	1.178	1.160	1.146	1.156	1.2	3.2	TM		
87	TM	4-Ethyltoluene	1.173	0.9909	1.012	1.065	1.034	1.080	1.086	1.056	1.072	1.1	4.9	TM		
88	TM	2-Chlorotoluene	1.032	1.018	0.9358	0.9070	0.9024	0.9205	0.8841	0.8629	0.7541	0.91	9.0	TM		
89	TM	1,3,5-Trimethylbenzene	1.111	1.007	0.9502	0.8656	1.004	1.040	1.002	0.9694	1.004	0.99	6.7	TM		
90	TM	4-Chlorotoluene	0.9827	0.9428	0.8406	0.9352	0.8957	0.9074	0.9014	0.8707	0.8848	0.91	4.6	TM		
91	TM	Tert-Butylbenzene	0.4821	0.4878	0.5201	0.4933	0.5732	0.5707	0.6035	0.5946	0.6177	0.55	9.8	TM		
92	TM	1,2,4-Trimethylbenzene	0.7998	0.9460	0.8049	0.9155	0.9690	0.9763	1.035	1.004	1.031	0.94	9.4	TM		
93	TM	Sec-Butylbenzene	1.011	0.9172	0.9188	1.056	1.073	1.105	1.121	1.107	1.151	1.1	8.1	TM		
94	TM	p-Isopropyltoluene		0.8303	0.8889	0.9044	1.049	1.057	1.118	1.118	1.161	1.0	12	TM		
95	TM	Benzyl Chloride	0.2242	0.2792	0.2661	0.2638	0.2167	0.2173	0.2234	0.2228	0.2515	0.24	10	TM		
96	TM	1,3-DCB	0.8194	0.6364	0.5705	0.6021	0.6799	0.6575	0.6709	0.6645	0.6786	0.66	10	TM		
97	TM	1,4-DCB	0.8033	0.7211	0.7006	0.5831	0.6388	0.6540	0.6682	0.6466	0.6748	0.68	9.1	TM		
98	TML	n-Butylbenzene	0.4112	0.4841	0.4046	0.4944	0.5656	0.5974	0.6856	0.7160	0.7902	0.57	24	TM	0.998	
99	TM	1,2-DCB	0.6692	0.6405	0.5987	0.6470	0.6582	0.6539	0.6635	0.6423	0.6804	0.65	3.6	TM		
100	TM	Hexachloroethane	0.1548	0.1591	0.2055	0.1841	0.1602	0.1575	0.1628	0.1663	0.1819	0.17	9.9	TM		
101	TML	1,2-Dibromo-3-chloropropane	0.0088	0.0293	0.0318	0.0402	0.0481	0.0559	0.0579	0.0579	0.0634	0.04	41	TM	0.999	
102	TML	1,2,4-Trichlorobenzene	0.1483	0.1203	0.1072	0.1196	0.1592	0.1983	0.2646	0.2864	0.3386	0.19	43	TM	0.995	
103	TML	Hexachlorobutadiene	0.2376	0.1684	0.1828	0.2143	0.2245	0.2533	0.2820	0.2891	0.3092	0.24	20	TM	0.999	
104	TMQ	Naphthalene	0.3645	0.2801	0.2235	0.2250	0.3044	0.4145	0.5147	0.6032	0.7496	0.41	44	TM	1.000	
105	TML	1,2,3-Trichlorobenzene	0.1506	0.1044	0.1263	0.1303	0.2031	0.2496	0.3344	0.3708	0.4644	0.24	54	TM	0.992	

Data File : M:\MAX\DATA\211015\1015M12.D
 Acq On : 15 Oct 21 15:12
 Sample : 0.3ug/L VOC STD 10/15/21
 Misc : IS&S 8/4/21

Vial: 2
 Operator: LP, DG, CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 13:28:38 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.34	96	397342	25.00	ppb	0.00
65) Chlorobenzene-D5 (IS)	9.50	117	352293	25.00	ppb	0.00
80) 1,4-Dichlorobenzene-D (IS)	11.82	152	217437	25.00	ppb	0.00

System Monitoring Compounds

41) Dibromofluoromethane (S)	5.56	111	28448	5.92	ppb	0.00
Spiked Amount				25.000		
			Recovery	=	23.696%	
46) 1,2-DCA-D4 (S)	5.95	65	20160	6.18	ppb	0.00
Spiked Amount				25.000		
			Recovery	=	24.716%	
66) Toluene-D8 (S)	8.05	98	94364	5.92	ppb	0.00
Spiked Amount				25.000		
			Recovery	=	23.668%	
74) 4-Bromofluorobenzene (S)	10.68	95	37378	5.45	ppb	0.00
Spiked Amount				25.000		
			Recovery	=	21.784%	

Target Compounds

	R.T.	QIon	Response	Conc	Units	Qvalue
2) Chlorotrifluoroethene	1.02	116	2364	15.17	ppb #	72
3) Dichlorodifluoromethane	1.19	85	437	0.22	ppb #	64
4) Freon 114	1.29	85	300	0.18	ppb #	59
5) Chloromethane	1.33	50	657	0.32	ppb #	81
6) Vinyl chloride	1.42	62	584	0.40	ppb #	61
7) 2-Chloro-1,1,1-trifluoroet	1.01	118	2099	48.48	ppb #	60
9) Chloroethane	1.80	64	445	0.36	ppb #	44
10) Dichlorofluoromethane	1.97	67	1225	0.36	ppb	93
11) Trichlorofluoromethane	2.01	101	1108	0.29	ppb	94
12) 2,2-Dichloro-1,1,1-trifluo.	2.21	85	45	37.16	ppb #	100
13) Acrolein	2.44	56	2646	7.09	ppb	94
14) Acetone	2.61	43	3165	6.98	ppb	98
15) Freon-113	2.54	151	532	0.30	ppb #	45
16) Acetonitrile	2.92	41	1607	12.67	ppb #	73
17) 2-propanol	2.28	45	21	1.12	ppb	92
18) 1,2-Dichlorotrifluoroethan	1.97	67	1225	0.36	ppb	100
19) 1,1-DCE	2.51	61	852	0.37	ppb #	84
20) t-Butanol	3.33	59	1829	6.84	ppb	100
21) Methyl Acetate	2.98	43	391	0.48	ppb #	49
22) Iodomethane	2.67	142	508	1.49	ppb #	65
23) Acrylonitrile	3.35	53	42	0.18	ppb #	21
25) Methylene chloride	3.08	84	716	0.43	ppb	98
26) Carbon disulfide	2.72	76	747	0.33	ppb #	82
27) Methyl t-butyl ether (MtBE)	3.46	73	1933	0.36	ppb #	58
28) Trans-1,2-DCE	3.44	96	316	-0.63	ppb #	66
29) 3-Methylpentane	3.50	57	383	-0.20	ppb #	14
30) Hexane	3.64	56	45	2.06	ppb	100

(#) = qualifier out of range (m) = manual integration

Data File : M:\MAX\DATA\211015\1015M12.D
 Acq On : 15 Oct 21 15:12
 Sample : 0.3ug/L VOC STD 10/15/21
 Misc : IS&S 8/4/21

Vial: 2
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 13:28:38 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
31) Diisopropyl Ether	4.25	45	817	0.22	ppb #	85
32) 1,1-DCA	4.07	63	636	0.23	ppb #	52
33) Vinyl Acetate	4.21	43	543	0.41	ppb #	77
34) Ethyl tert Butyl Ether	4.78	59	1368	0.28	ppb	93
35) Methylcyclopentane	4.75	56	20	0.10	ppb	100
36) MEK (2-Butanone)	4.98	43	2641	4.99	ppb #	85
37) Cis-1,2-DCE	4.91	96	719	0.37	ppb #	64
38) 2,2-Dichloropropane	4.88	77	1349	0.38	ppb #	61
39) Chloroform	5.36	83	741	0.20	ppb	79
40) Bromochloromethane	5.23	130	496	-0.43	ppb #	74
42) 1,1,1-TCA	5.54	97	1257	0.32	ppb #	75
43) Cyclohexane	5.57	41	375	0.32	ppb #	22
44) 1,1-Dichloropropene	5.74	75	630	0.28	ppb #	37
45) 2,2,4-Trimethylpentane	6.13	57	1141	0.32	ppb #	36
47) Carbon Tetrachloride	5.73	117	1289	0.36	ppb #	68
48) Tert Amyl Methyl Ether	6.18	73	1360	0.28	ppb #	91
49) 1,2-DCA	6.05	62	1047	0.31	ppb #	81
50) Benzene	5.99	78	2290	0.37	ppb #	84
51) TCE	6.75	95	606	-0.55	ppb #	79
52) 2-Pentanone	7.01	43	9248	10.52	ppb	94
54) Bromodichloromethane	7.31	83	707	0.24	ppb	90
55) Methyl Cyclohexane	6.94	83	946	-0.21	ppb #	70
56) Dibromomethane	7.12	93	450	0.40	ppb #	72
57) MIBK (methyl isobutyl ket	7.98	43	6119	5.11	ppb #	93
58) 1-Bromo-2-chloroethane	7.62	144	144	0.35	ppb #	15
59) 2-Chloroethyl vinyl ether	7.55	43	20	15.83	ppb #	100
60) Cis-1,3-Dichloropropene	7.79	75	576	0.21	ppb #	79
61) Toluene	8.12	91	2633	0.34	ppb	80
62) Trans-1,3-Dichloropropene	8.38	75	664	0.24	ppb #	29
63) 1,1,2-TCA	8.55	83	446	0.37	ppb #	57
64) 2-Hexanone	8.83	43	3704	4.34	ppb #	75
67) 1,2-EDB	9.03	107	473	0.30	ppb	100
68) Tetrachloroethene	8.66	164	2575	1.67	ppb #	81
69) 1-Chlorohexane	9.53	91	487	0.35	ppb	82
70) 1,1,1,2-Tetrachloroethane	9.61	131	588	0.23	ppb	78
71) m&p-Xylene	9.77	106	2405	0.62	ppb	90
72) o-Xylene	10.17	106	1391	0.36	ppb #	50
73) Styrene	10.18	104	1735	0.27	ppb #	81
75) 1,3-Dichloropropane	8.72	76	1057	0.44	ppb #	80
76) Dibromochloromethane	8.93	129	863	0.35	ppb #	72
77) Chlorobenzene	9.53	112	1915	0.32	ppb	91
78) Ethylbenzene	9.65	91	3451	0.39	ppb	91

(#) = qualifier out of range (m) = manual integration

Data File : M:\MAX\DATA\211015\1015M12.D
 Acq On : 15 Oct 21 15:12
 Sample : 0.3ug/L VOC STD 10/15/21
 Misc : IS&S 8/4/21

Vial: 2
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 13:28:38 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
79) Bromoform	10.35	173	759	0.37	ppb	89
81) Isopropylbenzene	10.53	105	3669	0.39	ppb	90
82) 1,1,2,2-Tetrachloroethane	10.84	83	842	0.53	ppb #	56
83) 1,2,3-Trichloropropane	10.88	110	81	-0.27	ppb #	6
84) t-1,4-Dichloro-2-Butene	10.91	53	354	1.04	ppb #	3
85) Bromobenzene	10.81	156	1060	0.33	ppb	76
86) n-Propylbenzene	10.94	91	3134	0.33	ppb	99
87) 4-Ethyltoluene	11.06	105	3060	0.34	ppb	92
88) 2-Chlorotoluene	11.02	91	2692	0.36	ppb	99
89) 1,3,5-Trimethylbenzene	11.13	105	2898	0.36	ppb	96
90) 4-Chlorotoluene	11.13	91	2564	0.34	ppb	89
91) Tert-Butylbenzene	11.45	119	1258	0.27	ppb	87
92) 1,2,4-Trimethylbenzene	11.48	105	2087	0.47	ppb	79
93) Sec-Butylbenzene	11.66	105	2637	0.31	ppb	97
94) p-Isopropyltoluene	11.81	119	1811	0.55	ppb #	62
95) Benzyl Chloride	11.99	91	585	0.27	ppb #	89
96) 1,3-DCB	11.76	146	2138	0.40	ppb	89
97) 1,4-DCB	11.85	146	2096	-0.11	ppb #	61
98) n-Butylbenzene	12.22	91	1073	1.08	ppb #	82
99) 1,2-DCB	12.22	146	1746	0.33	ppb #	84
100) Hexachloroethane	12.46	117	404	0.14	ppb #	66
101) 1,2-Dibromo-3-chloropropan	13.06	75	23	0.87	ppb #	1
102) 1,2,4-Trichlorobenzene	13.81	180	387	2.26	ppb #	70
103) Hexachlorobutadiene	13.99	225	620	1.04	ppb #	64
104) Naphthalene	14.05	128	951	0.77	ppb #	69
105) 1,2,3-Trichlorobenzene	14.30	180	393	3.03	ppb #	70

Quantitation Report


Data File : M:\MAX\DATA\211015\1015M12.D
 Acq On : 15 Oct 21 15:12
 Sample : 0.3ug/L VOC STD 10/15/21
 Misc : IS&S 8/4/21

Vial: 2
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 14:01:48 2021
 Response via : Initial Calibration

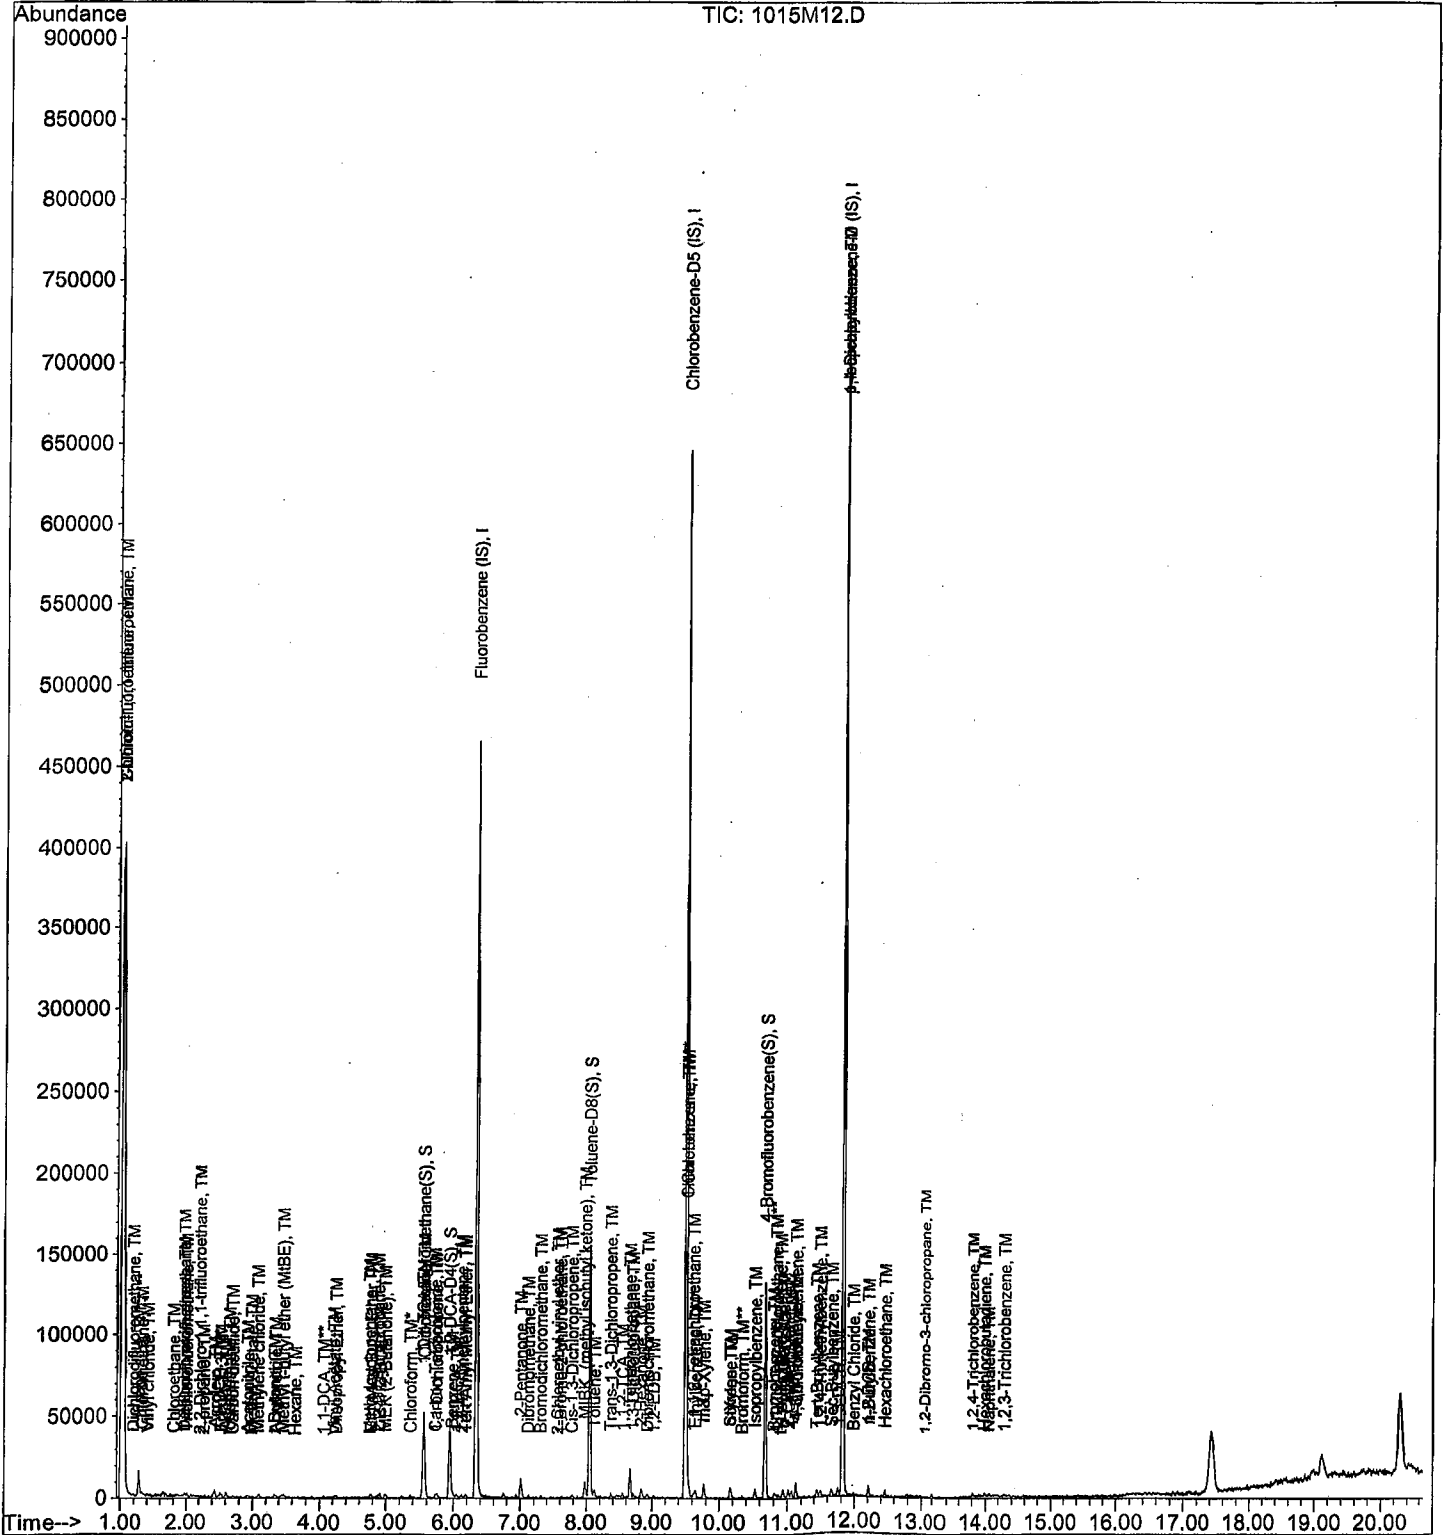

Data File : M:\MAX\DATA\211015\1015M13.D
 Acq On : 15 Oct 21 15:41
 Sample : 0.5ug/L VOC STD 10/15/21
 Misc : IS&S 8/4/21

Vial: 3
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 13:28:38 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.34	96	396824	25.00	ppb	0.00
65) Chlorobenzene-D5 (IS)	9.50	117	348546	25.00	ppb	0.00
80) 1,4-Dichlorobenzene-D (IS)	11.82	152	220294	25.00	ppb	0.00

System Monitoring Compounds

41) Dibromofluoromethane (S)	5.56	111	26504	5.53	ppb	0.00
Spiked Amount	25.000		Recovery	=	22.108%	
46) 1,2-DCA-D4 (S)	5.95	65	18016	5.53	ppb	0.00
Spiked Amount	25.000		Recovery	=	22.116%	
66) Toluene-D8 (S)	8.05	98	88728	5.62	ppb	0.00
Spiked Amount	25.000		Recovery	=	22.496%	
74) 4-Bromofluorobenzene (S)	10.68	95	32826	4.83	ppb	0.00
Spiked Amount	25.000		Recovery	=	19.340%	

Target Compounds

	R.T.	QIon	Response	Conc	Units	Qvalue
2) Chlorotrifluoroethene	1.02	116	1922	12.35	ppb	94
3) Dichlorodifluoromethane	1.19	85	1197	0.59	ppb	94
4) Freon 114	1.28	85	612	0.36	ppb	83
5) Chloromethane	1.33	50	648	0.31	ppb	91
6) Vinyl chloride	1.42	62	957	0.65	ppb	91
7) 2-Chloro-1,1,1-trifluoroet	1.01	118	2181	50.44	ppb #	40
8) Bromomethane	1.68	94	790	0.18	ppb	95
9) Chloroethane	1.78	64	763	0.68	ppb #	70
10) Dichlorofluoromethane	1.97	67	2477	0.74	ppb	87
11) Trichlorofluoromethane	2.00	101	2404	0.63	ppb	83
13) Acrolein	2.44	56	5714	15.34	ppb	85
14) Acetone	2.61	43	4830	10.67	ppb	100
15) Freon-113	2.52	151	1032	0.59	ppb #	76
16) Acetonitrile	2.93	41	2762	21.81	ppb	95
17) 2-propanol	2.24	45	71	3.78	ppb #	36
18) 1,2-Dichlorotrifluoroethan	1.97	67	2477	0.74	ppb	100
19) 1,1-DCE	2.51	61	1452	0.63	ppb #	80
20) t-Butanol	3.34	59	3416	24.57	ppb	100
21) Methyl Acetate	3.00	43	397	0.49	ppb #	26
22) Iodomethane	2.66	142	992	1.75	ppb #	91
23) Acrylonitrile	3.45	53	44	0.18	ppb #	21
24) 2-Methylpentane	2.05	71	22	9.10	ppb	100
25) Methylene chloride	3.08	84	819	0.49	ppb #	62
26) Carbon disulfide	2.71	76	1214	0.54	ppb #	76
27) Methyl t-butyl ether (MtBE)	3.47	73	3072	0.57	ppb	100
29) 3-Methylpentane	3.46	57	622	0.08	ppb #	88
31) Diisopropyl Ether	4.25	45	1808	0.49	ppb #	66

(#) = qualifier out of range (m) = manual integration

Data File : M:\MAX\DATA\211015\1015M13.D
 Acq On : 15 Oct 21 15:41
 Sample : 0.5ug/L VOC STD 10/15/21
 Misc : IS&S 8/4/21

Vial: 3
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 13:28:38 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
32) 1,1-DCA	4.05	63	1559	0.57	ppb	# 74
34) Ethyl tert Butyl Ether	4.77	59	2504	0.51	ppb	99
35) Methylcyclopentane	4.76	56	337	1.65	ppb	100
36) MEK (2-Butanone)	4.99	43	5170	9.78	ppb	# 82
37) Cis-1,2-DCE	4.91	96	1244	0.65	ppb	# 59
38) 2,2-Dichloropropane	4.89	77	1878	0.53	ppb	98
39) Chloroform	5.37	83	1603	0.43	ppb	89
40) Bromochloromethane	5.22	130	730	-0.26	ppb	# 78
42) 1,1,1-TCA	5.55	97	1922	0.49	ppb	# 85
43) Cyclohexane	5.58	41	660	0.56	ppb	# 25
44) 1,1-Dichloropropene	5.75	75	1253	0.56	ppb	# 53
45) 2,2,4-Trimethylpentane	6.11	57	1327	0.38	ppb	93
47) Carbon Tetrachloride	5.73	117	1862	0.52	ppb	93
48) Tert Amyl Methyl Ether	6.18	73	2629	0.55	ppb	93
49) 1,2-DCA	6.04	62	1754	0.51	ppb	# 90
50) Benzene	5.99	78	3585	0.57	ppb	# 79
51) TCE	6.75	95	1383	-0.12	ppb	# 62
52) 2-Pentanone	7.01	43	22294	25.38	ppb	99
53) 1,2-Dichloropropane	7.00	63	433	0.34	ppb	# 78
54) Bromodichloromethane	7.31	83	1703	0.58	ppb	76
55) Methyl Cyclohexane	6.94	83	1104	-0.14	ppb	89
56) Dibromomethane	7.13	93	651	0.58	ppb	# 59
57) MIBK (methyl isobutyl ket	7.98	43	10443	8.74	ppb	# 85
58) 1-Bromo-2-chloroethane	7.63	144	69	0.17	ppb	# 15
59) 2-Chloroethyl vinyl ether	7.72	43	20	15.85	ppb	# 100
60) Cis-1,3-Dichloropropene	7.79	75	1364	0.50	ppb	# 83
61) Toluene	8.12	91	3810	0.50	ppb	85
62) Trans-1,3-Dichloropropene	8.37	75	1104	0.39	ppb	# 67
63) 1,1,2-TCA	8.55	83	763	0.63	ppb	# 68
64) 2-Hexanone	8.83	43	6286	7.37	ppb	# 75
67) 1,2-EDB	9.03	107	1108	0.71	ppb	# 61
68) Tetrachloroethene	8.66	164	2429	1.59	ppb	# 78
69) 1-Chlorohexane	9.53	91	621	0.45	ppb	86
70) 1,1,1,2-Tetrachloroethane	9.62	131	1274	0.50	ppb	97
71) m&p-Xylene	9.77	106	3509	0.92	ppb	76
72) o-Xylene	10.16	106	2198	0.57	ppb	64
73) Styrene	10.18	104	2988	0.47	ppb	87
75) 1,3-Dichloropropane	8.72	76	1283	0.54	ppb	100
76) Dibromochloromethane	8.94	129	1320	0.55	ppb	87
77) Chlorobenzene	9.53	112	2829	0.48	ppb	# 87
78) Ethylbenzene	9.65	91	4309	0.49	ppb	97
79) Bromoform	10.35	173	870	0.43	ppb	86

(#) = qualifier out of range (m) = manual integration

Data File : M:\MAX\DATA\211015\1015M13.D
 Acq On : 15 Oct 21 15:41
 Sample : 0.5ug/L VOC STD 10/15/21
 Misc : IS&S 8/4/21

Vial: 3
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 13:28:38 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
81) Isopropylbenzene	10.53	105	5427	0.56	ppb	97
82) 1,1,2,2-Tetrachloroethane	10.84	83	1084	0.67	ppb #	62
83) 1,2,3-Trichloropropane	10.88	110	484	0.27	ppb #	79
84) t-1,4-Dichloro-2-Butene	10.91	53	123	0.57	ppb #	3
85) Bromobenzene	10.82	156	1801	0.55	ppb	93
86) n-Propylbenzene	10.95	91	5177	0.54	ppb	100
87) 4-Ethyltoluene	11.06	105	4366	0.48	ppb #	82
88) 2-Chlorotoluene	11.02	91	4485	0.60	ppb	89
89) 1,3,5-Trimethylbenzene	11.12	105	4437	0.54	ppb	86
90) 4-Chlorotoluene	11.12	91	4154	0.55	ppb	95
91) Tert-Butylbenzene	11.45	119	2149	0.46	ppb	95
92) 1,2,4-Trimethylbenzene	11.49	105	4168	0.72	ppb	83
93) Sec-Butylbenzene	11.66	105	4041	0.47	ppb	91
94) p-Isopropyltoluene	11.81	119	3658	0.74	ppb	95
95) Benzyl Chloride	12.00	91	1230	0.56	ppb #	84
96) 1,3-DCB	11.76	146	2804	0.52	ppb #	85
97) 1,4-DCB	11.85	146	3177	0.09	ppb	93
98) n-Butylbenzene	12.21	91	2133	1.25	ppb	87
99) 1,2-DCB	12.21	146	2822	0.53	ppb #	84
100) Hexachloroethane	12.45	117	701	0.35	ppb #	51
101) 1,2-Dibromo-3-chloropropan	12.99	75	129	1.10	ppb #	1
102) 1,2,4-Trichlorobenzene	13.82	180	530	2.32	ppb #	45
103) Hexachlorobutadiene	13.99	225	742	1.09	ppb #	82
104) Naphthalene	14.05	128	1234	0.86	ppb #	69
105) 1,2,3-Trichlorobenzene	14.30	180	460	3.05	ppb #	69

Quantitation Report


Data File : M:\MAX\DATA\211015\1015M13.D
Acq On : 15 Oct 21 15:41
Sample : 0.5ug/L VOC STD 10/15/21
Misc : IS&S 8/4/21

Vial: 3
Operator: LP,DG,CH
Inst : Max
Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
Title : METHOD 8260B
Last Update : Sat Oct 16 14:01:48 2021
Response via : Initial Calibration

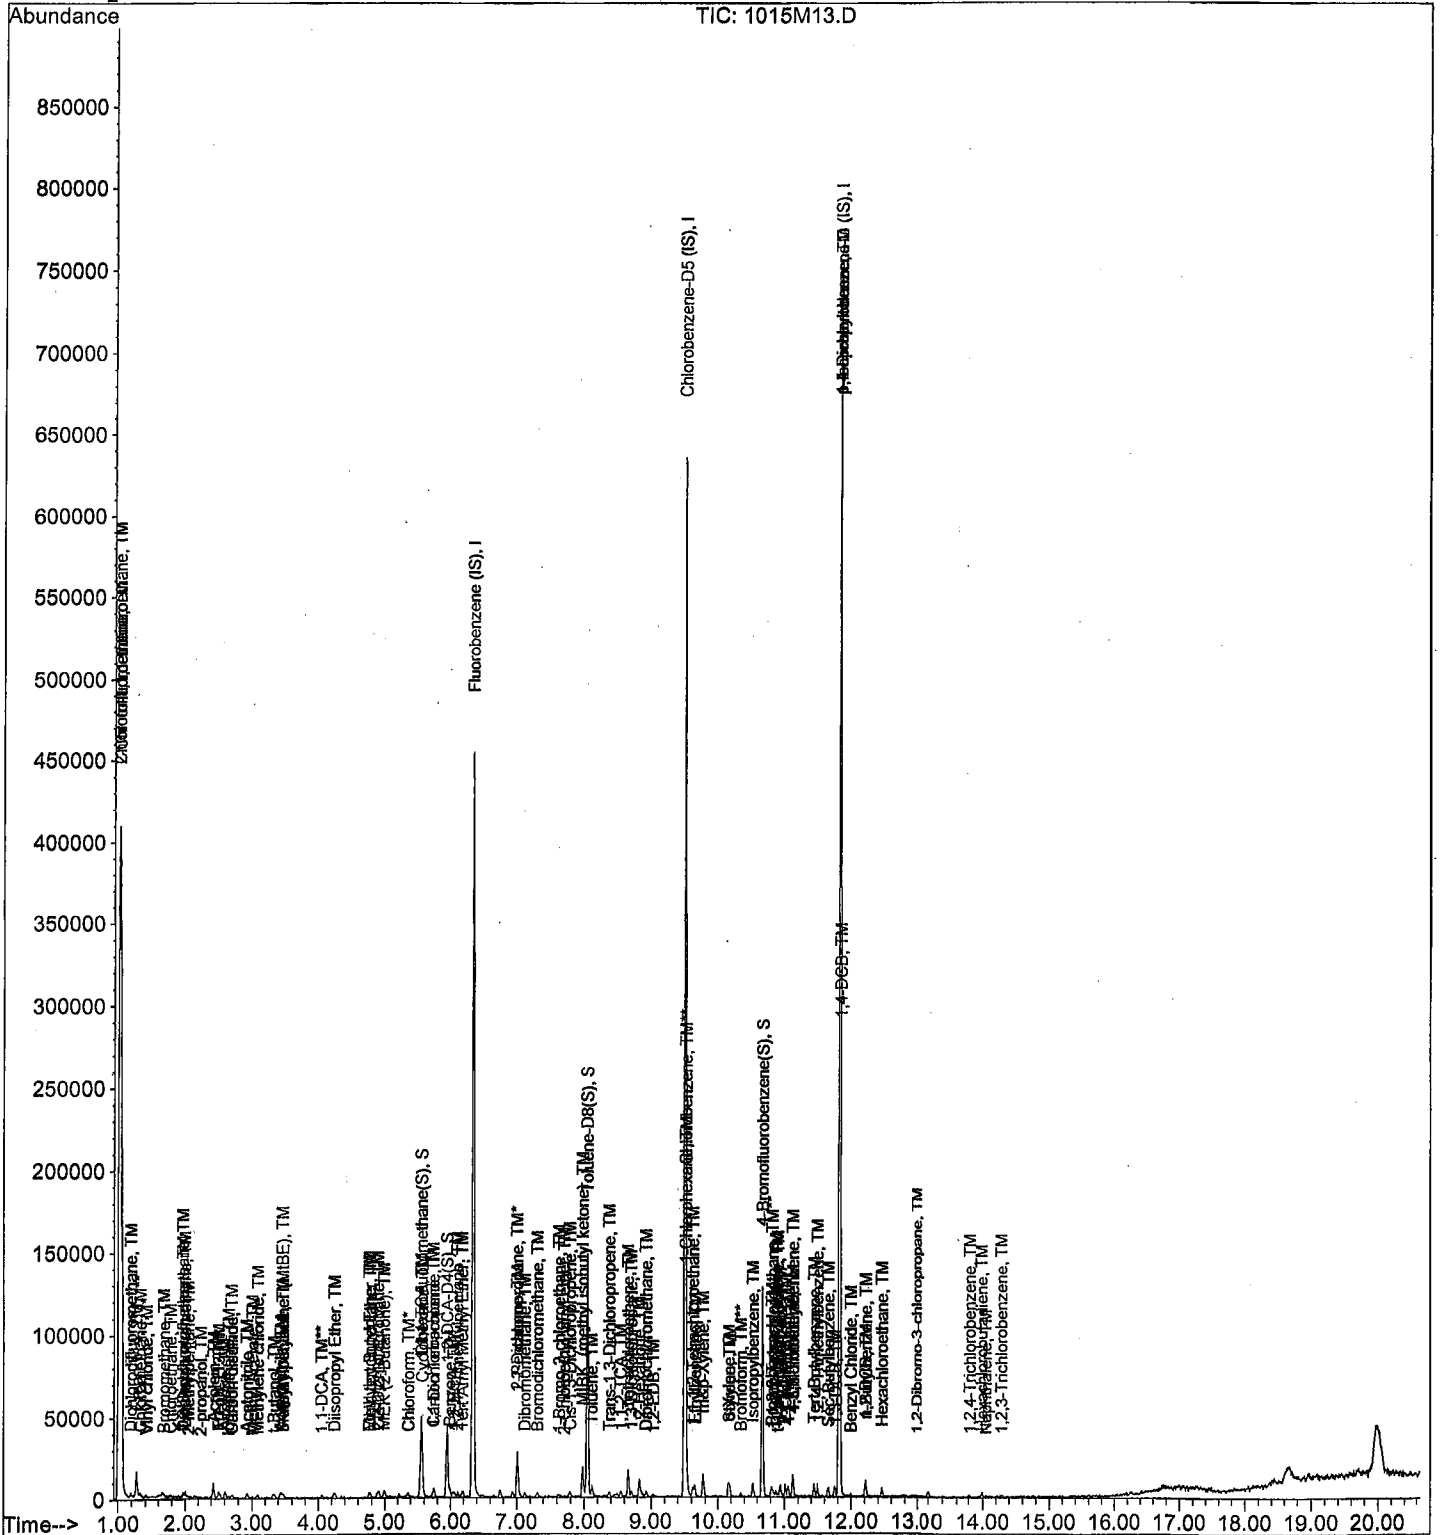

Data File : M:\MAX\DATA\211015\1015M14.D
 Acq On : 15 Oct 21 16:09
 Sample : 1ug/L VOC STD 10/15/21
 Misc : IS&S 8/4/21

Vial: 4
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 13:28:38 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.34	96	394605	25.00	ppb	0.00
65) Chlorobenzene-D5 (IS)	9.50	117	355921	25.00	ppb	0.00
80) 1,4-Dichlorobenzene-D (IS)	11.82	152	218264	25.00	ppb	0.00
System Monitoring Compounds						
41) Dibromofluoromethane(S)	5.56	111	47945	10.05	ppb	0.00
Spiked Amount				Recovery =	40.216%	
46) 1,2-DCA-D4(S)	5.95	65	33328	10.29	ppb	0.00
Spiked Amount				Recovery =	41.144%	
66) Toluene-D8(S)	8.05	98	157547	9.78	ppb	0.00
Spiked Amount				Recovery =	39.116%	
74) 4-Bromofluorobenzene(S)	10.68	95	61144	8.82	ppb	0.00
Spiked Amount				Recovery =	35.276%	
Target Compounds						
2) Chlorotrifluoroethene	1.01	116	1602	10.35	ppb #	12
3) Dichlorodifluoromethane	1.19	85	2543	1.27	ppb	91
4) Freon 114	1.29	85	1368	0.81	ppb	78
5) Chloromethane	1.33	50	1636	1.13	ppb	90
6) Vinyl chloride	1.42	62	1546	1.05	ppb #	78
7) 2-Chloro-1,1,1-trifluoroet	1.01	118	2765	64.30	ppb #	65
8) Bromomethane	1.68	94	1565	0.99	ppb	84
9) Chloroethane	1.78	64	2493	2.43	ppb	94
10) Dichlorofluoromethane	1.97	67	4092	1.22	ppb #	80
11) Trichlorofluoromethane	2.00	101	4558	1.21	ppb	84
12) 2,2-Dichloro-1,1,1-trifluo	2.40	85	21	17.46	ppb	100
13) Acrolein	2.43	56	10691	28.86	ppb	94
14) Acetone	2.61	43	10882	24.17	ppb	89
15) Freon-113	2.53	151	2046	1.17	ppb #	88
16) Acetonitrile	2.92	41	5855	46.50	ppb #	94
17) 2-propanol	2.26	45	136	7.29	ppb #	83
18) 1,2-Dichlorotrifluoroethan	1.97	67	4092	1.22	ppb	100
19) 1,1-DCE	2.51	61	2994	1.31	ppb #	89
20) t-Butanol	3.34	59	7682	57.57	ppb	98
21) Methyl Acetate	3.00	43	760	0.94	ppb	87
22) Iodomethane	2.66	142	1392	1.97	ppb #	86
23) Acrylonitrile	3.43	53	471	1.12	ppb #	42
25) Methylene chloride	3.08	84	1772	1.07	ppb	86
26) Carbon disulfide	2.72	76	2194	0.99	ppb #	87
27) Methyl t-butyl ether (MtBE)	3.47	73	6302	1.18	ppb	98
28) Trans-1,2-DCE	3.43	96	1741	0.31	ppb	80
29) 3-Methylpentane	3.34	57	1128	0.68	ppb #	72

(#) = qualifier out of range (m) = manual integration

Data File : M:\MAX\DATA\211015\1015M14.D
 Acq On : 15 Oct 21 16:09
 Sample : 1ug/L VOC STD 10/15/21
 Misc : IS&S 8/4/21

Vial: 4
 Operator: LP, DG, CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 13:28:38 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
31) Diisopropyl Ether	4.25	45	3947	1.07	ppb	# 82
32) 1,1-DCA	4.05	63	3272	1.19	ppb	# 79
34) Ethyl tert Butyl Ether	4.78	59	4498	0.93	ppb	# 61
35) Methylcyclopentane	4.77	56	269	1.32	ppb	100
36) MEK (2-Butanone)	4.99	43	11464	21.80	ppb	86
37) Cis-1,2-DCE	4.92	96	2282	1.19	ppb	75
38) 2,2-Dichloropropane	4.90	77	3468	0.98	ppb	# 85
39) Chloroform	5.36	83	3948	1.05	ppb	89
40) Bromochloromethane	5.23	130	1469	0.28	ppb	# 84
42) 1,1,1-TCA	5.54	97	4273	1.09	ppb	# 84
43) Cyclohexane	5.59	41	1433	1.22	ppb	# 68
44) 1,1-Dichloropropene	5.74	75	2385	1.08	ppb	94
45) 2,2,4-Trimethylpentane	6.11	57	3345	0.96	ppb	# 69
47) Carbon Tetrachloride	5.73	117	4212	1.19	ppb	82
48) Tert Amyl Methyl Ether	6.18	73	4217	0.88	ppb	# 95
49) 1,2-DCA	6.04	62	3756	1.10	ppb	# 81
50) Benzene	6.00	78	6941	1.11	ppb	# 82
51) TCE	6.75	95	2471	0.48	ppb	89
52) 2-Pentanone	7.01	43	44308	50.73	ppb	100
53) 1,2-Dichloropropane	7.00	63	811	0.93	ppb	# 45
54) Bromodichloromethane	7.31	83	2624	0.90	ppb	95
55) Methyl Cyclohexane	6.94	83	2273	0.38	ppb	76
56) Dibromomethane	7.12	93	1650	1.48	ppb	# 63
57) MIBK (methyl isobutyl ket	7.98	43	22869	19.25	ppb	94
58) 1-Bromo-2-chloroethane	7.63	144	263	0.64	ppb	# 15
59) 2-Chloroethyl vinyl ether	7.56	43	22	17.53	ppb	# 100
60) Cis-1,3-Dichloropropene	7.79	75	2697	0.99	ppb	94
61) Toluene	8.12	91	7543	0.99	ppb	88
62) Trans-1,3-Dichloropropene	8.37	75	2660	0.95	ppb	96
63) 1,1,2-TCA	8.56	83	1005	0.84	ppb	84
64) 2-Hexanone	8.83	43	15739	18.57	ppb	97
67) 1,2-EDB	9.03	107	1731	1.09	ppb	84
68) Tetrachloroethene	8.66	164	3240	2.08	ppb	85
69) 1-Chlorohexane	9.53	91	1541	1.09	ppb	96
70) 1,1,1,2-Tetrachloroethane	9.62	131	2346	0.90	ppb	78
71) m&p-Xylene	9.77	106	7601	1.95	ppb	79
72) o-Xylene	10.16	106	4468	1.13	ppb	# 50
73) Styrene	10.18	104	5452	0.84	ppb	97
75) 1,3-Dichloropropane	8.72	76	2708	1.11	ppb	# 79
76) Dibromochloromethane	8.93	129	2732	1.11	ppb	84
77) Chlorobenzene	9.52	112	5459	0.91	ppb	89
78) Ethylbenzene	9.65	91	9241	1.02	ppb	98

Data File : M:\MAX\DATA\211015\1015M14.D
 Acq On : 15 Oct 21 16:09
 Sample : 1ug/L VOC STD 10/15/21
 Misc : IS&S 8/4/21

Vial: 4
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 13:28:38 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
79) Bromoform	10.35	173	2258	1.10	ppb	98
81) Isopropylbenzene	10.53	105	9854	1.03	ppb	90
82) 1,1,2,2-Tetrachloroethane	10.84	83	1852	1.16	ppb #	71
83) 1,2,3-Trichloropropane	10.88	110	827	0.74	ppb	84
84) t-1,4-Dichloro-2-Butene	10.89	53	653	1.64	ppb #	37
85) Bromobenzene	10.81	156	3021	0.93	ppb	97
86) n-Propylbenzene	10.94	91	9945	1.04	ppb	98
87) 4-Ethyltoluene	11.06	105	8835	0.99	ppb #	81
88) 2-Chlorotoluene	11.01	91	8170	1.10	ppb	86
89) 1,3,5-Trimethylbenzene	11.13	105	8296	1.01	ppb #	76
90) 4-Chlorotoluene	11.13	91	7339	0.98	ppb	93
91) Tert-Butylbenzene	11.44	119	4541	0.98	ppb	91
92) 1,2,4-Trimethylbenzene	11.49	105	7027	1.07	ppb	97
93) Sec-Butylbenzene	11.66	105	8022	0.93	ppb	99
94) p-Isopropyltoluene	11.81	119	7761	1.20	ppb	94
95) Benzyl Chloride	11.99	91	2323	1.07	ppb	92
96) 1,3-DCB	11.76	146	4981	0.93	ppb	94
97) 1,4-DCB	11.84	146	6117	0.68	ppb	86
98) n-Butylbenzene	12.21	91	3532	1.48	ppb	84
99) 1,2-DCB	12.21	146	5227	0.99	ppb	95
100) Hexachloroethane	12.46	117	1794	1.13	ppb	73
101) 1,2-Dibromo-3-chloropropan	13.00	75	278	1.43	ppb #	59
102) 1,2,4-Trichlorobenzene	13.81	180	936	2.49	ppb	88
103) Hexachlorobutadiene	13.98	225	1596	1.44	ppb	91
104) Naphthalene	14.06	128	1951	1.11	ppb #	92
105) 1,2,3-Trichlorobenzene	14.29	180	1103	3.26	ppb #	74

Quantitation Report


Data File : M:\MAX\DATA\211015\1015M14.D
Acq On : 15 Oct 21 16:09
Sample : 1ug/L VOC STD 10/15/21
Misc : IS&S 8/4/21

Vial: 4
Operator: LP,DG,CH
Inst : Max
Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
Title : METHOD 8260B
Last Update : Sat Oct 16 14:01:48 2021
Response via : Initial Calibration

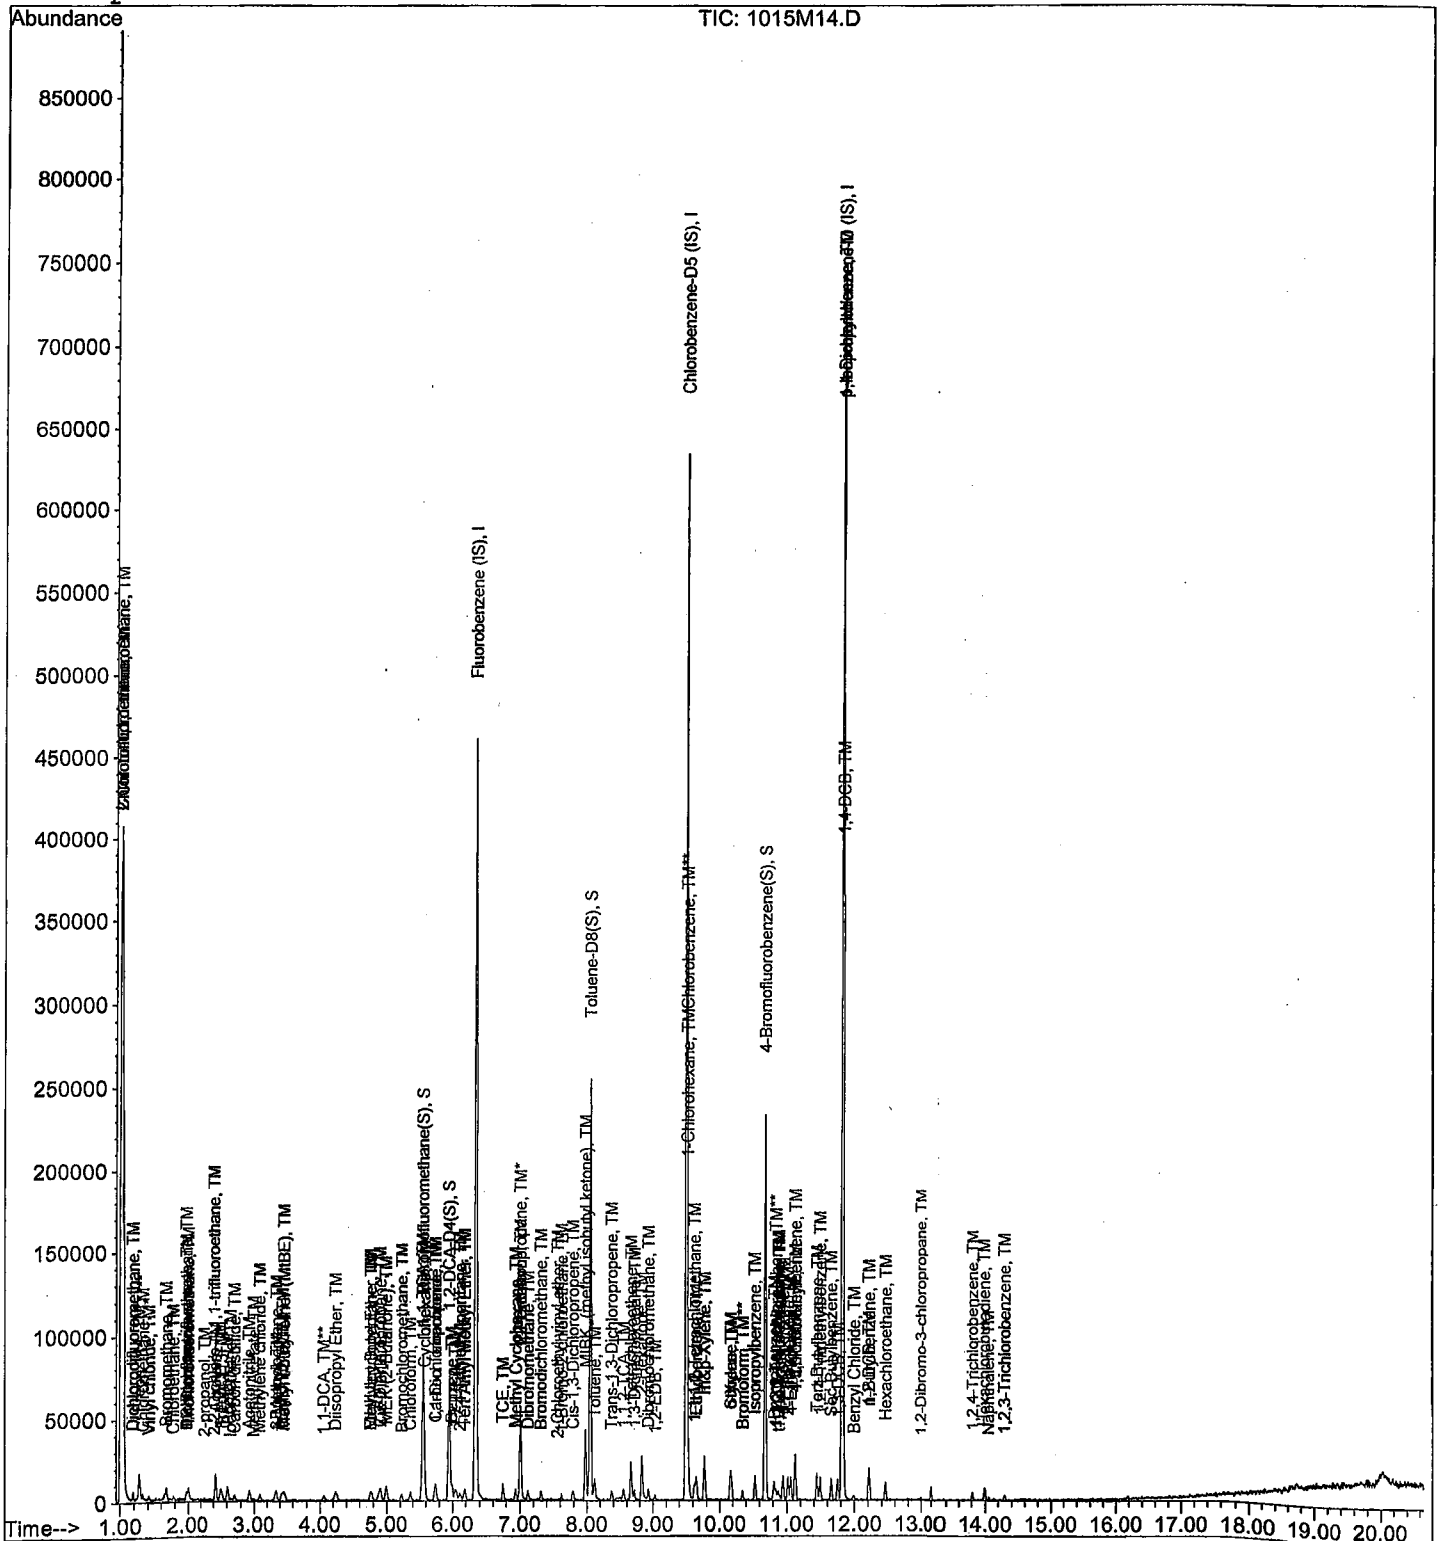

Data File : M:\MAX\DATA\211015\1015M15.D
 Acq On : 15 Oct 21 16:38
 Sample : 2ug/L VOC STD 10/15/21
 Misc : IS&S 8/4/21

Vial: 5
 Operator: LP, DG, CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 13:28:38 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.34	96	397741	25.00	ppb	0.00
65) Chlorobenzene-D5 (IS)	9.50	117	352458	25.00	ppb	0.00
80) 1,4-Dichlorobenzene-D (IS)	11.82	152	222724	25.00	ppb	0.00

System Monitoring Compounds

41) Dibromofluoromethane(S)	5.56	111	46784	9.73	ppb	0.00
Spiked Amount	25.000		Recovery	=	38.932%	
46) 1,2-DCA-D4(S)	5.95	65	32664	10.00	ppb	0.00
Spiked Amount	25.000		Recovery	=	40.008%	
66) Toluene-D8(S)	8.05	98	156127	9.79	ppb	0.00
Spiked Amount	25.000		Recovery	=	39.144%	
74) 4-Bromofluorobenzene(S)	10.68	95	61174	8.91	ppb	0.00
Spiked Amount	25.000		Recovery	=	35.640%	

Target Compounds

	R.T.	QIon	Response	Conc	Units	Qvalue
2) Chlorotrifluoroethene	1.02	116	2218	14.22	ppb	# 51
3) Dichlorodifluoromethane	1.18	85	4500	2.23	ppb	98
4) Freon 114	1.29	85	2873	1.69	ppb	80
5) Chloromethane	1.33	50	2712	2.00	ppb	# 86
6) Vinyl chloride	1.42	62	3230	2.18	ppb	92
7) 2-Chloro-1,1,1-trifluoroet	1.02	118	1945	44.88	ppb	# 38
8) Bromomethane	1.68	94	2697	2.14	ppb	95
9) Chloroethane	1.78	64	1755	1.67	ppb	# 67
10) Dichlorofluoromethane	1.97	67	6925	2.05	ppb	94
11) Trichlorofluoromethane	2.00	101	9973	2.63	ppb	98
13) Acrolein	2.43	56	18305	49.03	ppb	98
14) Acetone	2.61	43	15819	34.86	ppb	94
15) Freon-113	2.52	151	3875	2.20	ppb	# 85
16) Acetonitrile	2.93	41	8400	66.18	ppb	96
17) 2-propanol	2.25	45	148	7.87	ppb	# 55
18) 1,2-Dichlorotrifluoroethan	1.97	67	6925	2.05	ppb	100
19) 1,1-DCE	2.51	61	5750	2.49	ppb	90
20) t-Butanol	3.34	59	12116	82.21	ppb	99
21) Methyl Acetate	2.99	43	1802	2.21	ppb	91
22) Iodomethane	2.66	142	2280	2.44	ppb	# 85
23) Acrylonitrile	3.43	53	760	1.75	ppb	96
24) 2-Methylpentane	2.29	71	46	18.97	ppb	100
25) Methylene chloride	3.08	84	3477	2.07	ppb	93
26) Carbon disulfide	2.71	76	5106	2.28	ppb	97
27) Methyl t-butyl ether (MtBE)	3.46	73	11162	2.07	ppb	# 87
28) Trans-1,2-DCE	3.43	96	3660	1.56	ppb	86
29) 3-Methylpentane	3.47	57	2566	2.34	ppb	# 92

(#) = qualifier out of range (m) = manual integration

Data File : M:\MAX\DATA\211015\1015M15.D
 Acq On : 15 Oct 21 16:38
 Sample : 2ug/L VOC STD 10/15/21
 Misc : IS&S 8/4/21

Vial: 5
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 13:28:38 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
31) Diisopropyl Ether	4.25	45	7913	2.12	ppb	# 71
32) 1,1-DCA	4.06	63	5912	2.14	ppb	# 91
34) Ethyl tert Butyl Ether	4.77	59	9568	1.96	ppb	91
35) Methylcyclopentane	4.78	56	494	2.41	ppb	100
36) MEK (2-Butanone)	4.99	43	16761	31.63	ppb	# 85
37) Cis-1,2-DCE	4.91	96	3543	1.84	ppb	76
38) 2,2-Dichloropropane	4.89	77	6978	1.95	ppb	98
39) Chloroform	5.36	83	7578	2.00	ppb	97
40) Bromochloromethane	5.22	130	3743	1.92	ppb	# 79
42) 1,1,1-TCA	5.54	97	9181	2.32	ppb	92
43) Cyclohexane	5.59	41	2567	2.16	ppb	93
44) 1,1-Dichloropropene	5.75	75	4670	2.10	ppb	98
45) 2,2,4-Trimethylpentane	6.11	57	7204	2.04	ppb	# 50
47) Carbon Tetrachloride	5.73	117	8319	2.33	ppb	82
48) Tert Amyl Methyl Ether	6.18	73	9116	1.89	ppb	# 93
49) 1,2-DCA	6.04	62	7832	2.28	ppb	# 87
50) Benzene	5.99	78	13478	2.15	ppb	94
51) TCE	6.75	95	4321	1.48	ppb	92
52) 2-Pentanone	7.01	43	68287	77.56	ppb	94
53) 1,2-Dichloropropane	7.01	63	1147	1.43	ppb	# 78
54) Bromodichloromethane	7.31	83	6459	2.21	ppb	94
55) Methyl Cyclohexane	6.94	83	5097	1.61	ppb	97
56) Dibromomethane	7.12	93	2762	2.46	ppb	# 77
57) MIBK (methyl isobutyl ket	7.98	43	36816	30.74	ppb	97
58) 1-Bromo-2-chloroethane	7.63	144	737	1.77	ppb	75
59) 2-Chloroethyl vinyl ether	7.81	43	19	15.02	ppb	# 100
60) Cis-1,3-Dichloropropene	7.79	75	6027	2.19	ppb	91
61) Toluene	8.12	91	15184	1.97	ppb	85
62) Trans-1,3-Dichloropropene	8.38	75	5713	2.03	ppb	86
63) 1,1,2-TCA	8.54	83	2414	1.99	ppb	93
64) 2-Hexanone	8.83	43	24259	28.40	ppb	97
67) 1,2-EDB	9.03	107	3866	2.45	ppb	83
68) Tetrachloroethene	8.66	164	4952	3.20	ppb	# 80
69) 1-Chlorohexane	9.53	91	2721	1.95	ppb	# 79
70) 1,1,1,2-Tetrachloroethane	9.62	131	5242	2.02	ppb	90
71) m&p-Xylene	9.77	106	15266	3.95	ppb	88
72) o-Xylene	10.16	106	7227	1.84	ppb	97
73) Styrene	10.18	104	12118	1.89	ppb	99
75) 1,3-Dichloropropane	8.71	76	5024	2.07	ppb	90
76) Dibromochloromethane	8.93	129	5242	2.15	ppb	94
77) Chlorobenzene	9.53	112	12976	2.19	ppb	90
78) Ethylbenzene	9.65	91	18350	2.05	ppb	96

Data File : M:\MAX\DATA\211015\1015M15.D
 Acq On : 15 Oct 21 16:38
 Sample : 2ug/L VOC STD 10/15/21
 Misc : IS&S 8/4/21

Vial: 5
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 13:28:38 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
79) Bromoform	10.35	173	4619	2.28	ppb	87
81) Isopropylbenzene	10.53	105	18752	1.93	ppb	92
82) 1,1,2,2-Tetrachloroethane	10.84	83	3694	2.26	ppb	93
83) 1,2,3-Trichloropropane	10.87	110	1874	2.10	ppb #	77
84) t-1,4-Dichloro-2-Butene	10.90	53	1005	2.32	ppb	98
85) Bromobenzene	10.81	156	7210	2.17	ppb	90
86) n-Propylbenzene	10.94	91	19095	1.96	ppb	99
87) 4-Ethyltoluene	11.06	105	18983	2.08	ppb	92
88) 2-Chlorotoluene	11.02	91	16161	2.13	ppb	90
89) 1,3,5-Trimethylbenzene	11.12	105	15423	1.85	ppb	93
90) 4-Chlorotoluene	11.13	91	16663	2.18	ppb	98
91) Tert-Butylbenzene	11.44	119	8790	1.86	ppb	92
92) 1,2,4-Trimethylbenzene	11.49	105	16313	2.15	ppb	86
93) Sec-Butylbenzene	11.66	105	18809	2.14	ppb	99
94) p-Isopropyltoluene	11.81	119	16115	2.08	ppb	90
95) Benzyl Chloride	12.00	91	4701	2.12	ppb	96
96) 1,3-DCB	11.75	146	10728	1.97	ppb #	93
97) 1,4-DCB	11.84	146	10390	1.48	ppb #	80
98) n-Butylbenzene	12.22	91	8810	2.32	ppb	94
99) 1,2-DCB	12.21	146	11528	2.15	ppb	96
100) Hexachloroethane	12.45	117	3280	2.14	ppb	90
101) 1,2-Dibromo-3-chloropropan	13.00	75	716	2.35	ppb #	72
102) 1,2,4-Trichlorobenzene	13.81	180	2131	2.97	ppb #	84
103) Hexachlorobutadiene	13.99	225	3819	2.33	ppb	82
104) Naphthalene	14.05	128	4009	1.77	ppb #	88
105) 1,2,3-Trichlorobenzene	14.29	180	2322	3.64	ppb	94

Quantitation Report


Data File : M:\MAX\DATA\211015\1015M15.D
Acq On : 15 Oct 21 16:38
Sample : 2ug/L VOC STD 10/15/21
Misc : IS&S 8/4/21

Vial: 5
Operator: LP,DG,CH
Inst : Max
Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
Title : METHOD 8260B
Last Update : Sat Oct 16 14:01:48 2021
Response via : Initial Calibration

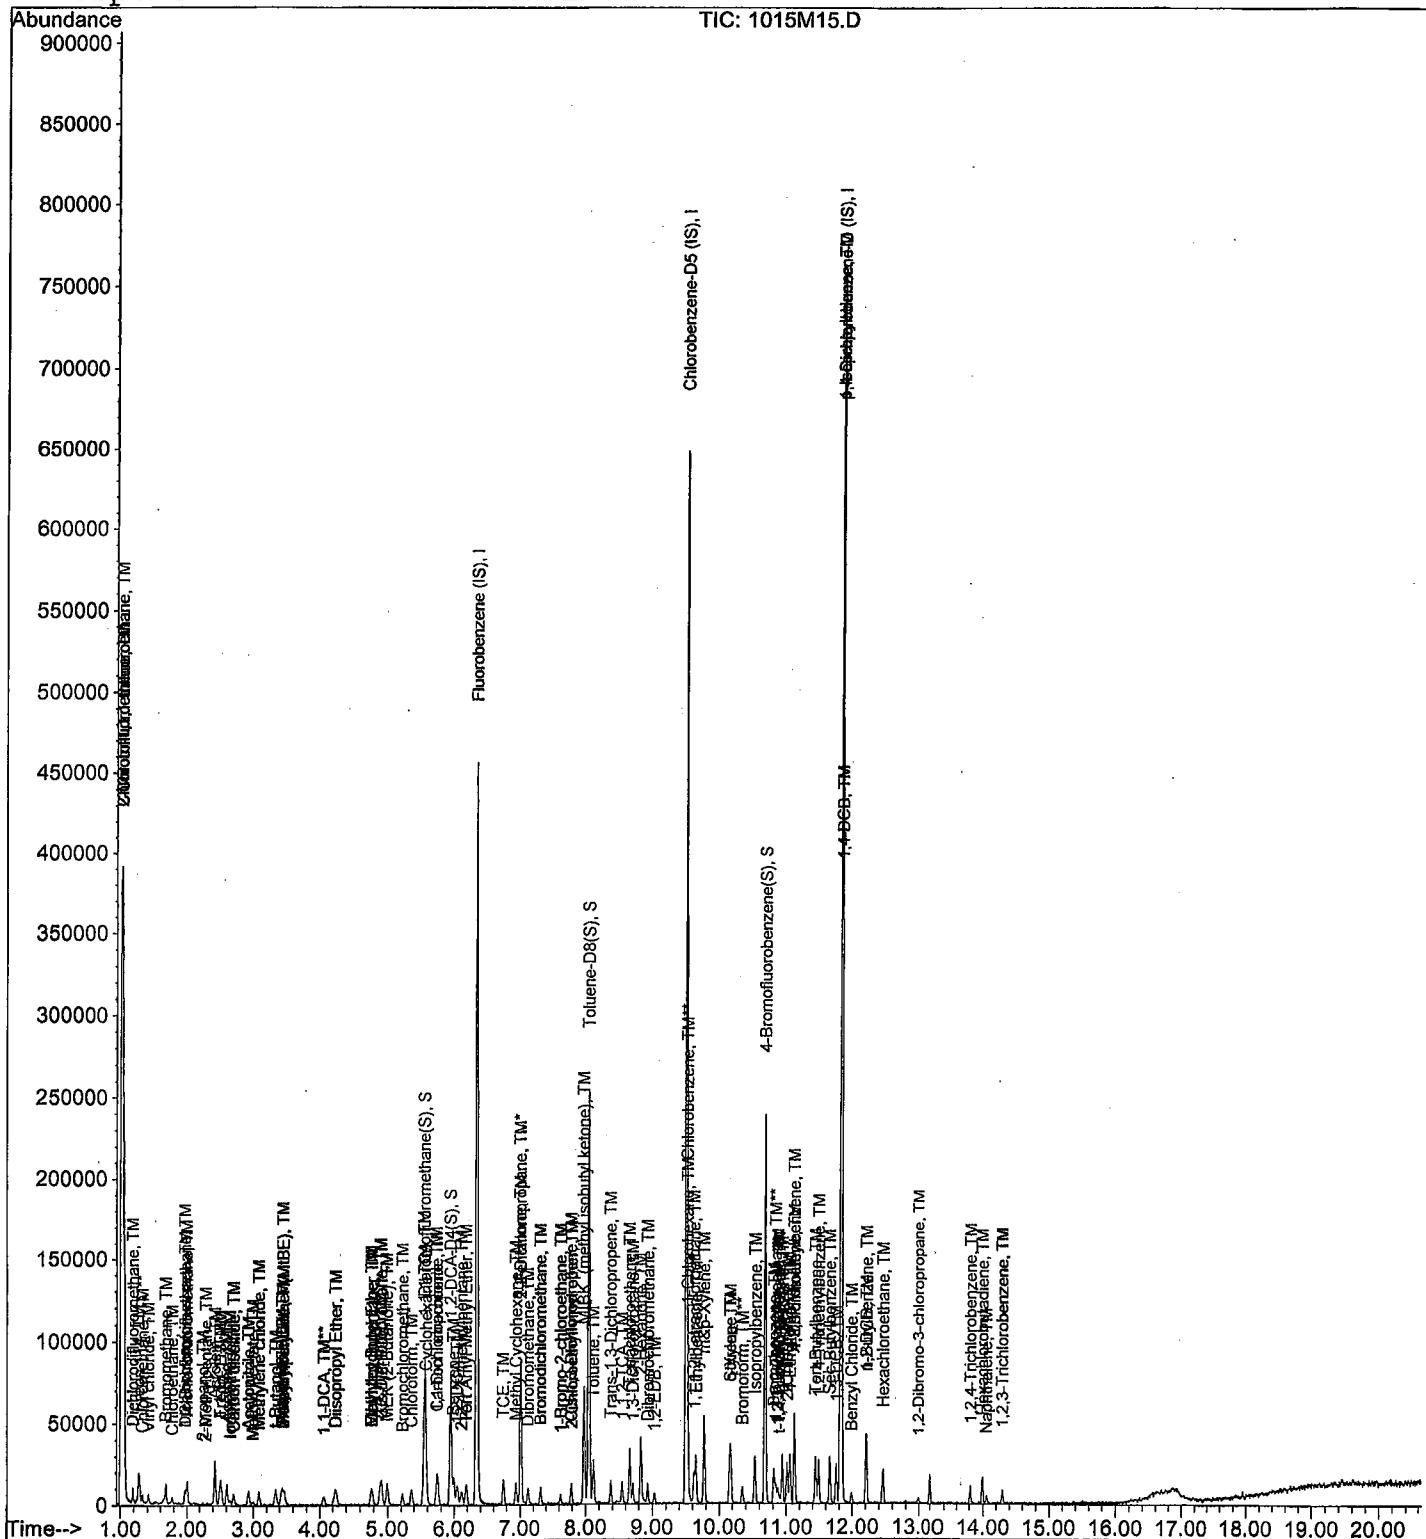

Data File : M:\MAX\DATA\211015\1015M16.D
 Acq On : 15 Oct 21 17:06
 Sample : 5ug/L VOC STD 10/15/21
 Misc : IS&S 8/4/21

Vial: 6
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 13:28:38 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.34	96	387411	25.00	ppb	0.00
65) Chlorobenzene-D5 (IS)	9.50	117	344894	25.00	ppb	0.00
80) 1,4-Dichlorobenzene-D (IS)	11.82	152	232454	25.00	ppb	0.00
System Monitoring Compounds						
41) Dibromofluoromethane(S)	5.56	111	118038	25.21	ppb	0.00
Spiked Amount	25.000		Recovery	=	100.844%	
46) 1,2-DCA-D4 (S)	5.95	65	84056	26.42	ppb	0.00
Spiked Amount	25.000		Recovery	=	105.700%	
66) Toluene-D8 (S)	8.05	98	389321	24.94	ppb	0.00
Spiked Amount	25.000		Recovery	=	99.748%	
74) 4-Bromofluorobenzene(S)	10.68	95	156913	23.35	ppb	0.00
Spiked Amount	25.000		Recovery	=	93.416%	
Target Compounds						
2) Chlorotrifluoroethene	1.02	116	1951	12.84	ppb	92
3) Dichlorodifluoromethane	1.18	85	13541	6.89	ppb	91
4) Freon 114	1.29	85	6948	4.20	ppb	87
5) Chloromethane	1.33	50	7282	5.89	ppb	# 83
6) Vinyl chloride	1.42	62	8698	6.04	ppb	97
7) 2-Chloro-1,1,1-trifluoroet	1.01	118	2807	66.49	ppb	# 56
8) Bromomethane	1.68	94	7347	7.13	ppb	89
9) Chloroethane	1.77	64	5473	5.54	ppb	90
10) Dichlorofluoromethane	1.97	67	17069	5.20	ppb	93
11) Trichlorofluoromethane	2.00	101	23038	6.23	ppb	98
13) Acrolein	2.43	56	21061	57.91	ppb	97
14) Acetone	2.61	43	19225	43.50	ppb	100
15) Freon-113	2.53	151	8907	5.20	ppb	89
16) Acetonitrile	2.92	41	11772	95.23	ppb	97
17) 2-propanol	2.26	45	534	29.16	ppb	# 83
18) 1,2-Dichlorotrifluoroethan	1.97	67	17069	5.20	ppb	100
19) 1,1-DCE	2.51	61	13232	5.88	ppb	96
20) t-Butanol	3.34	59	16999	106.77	ppb	95
21) Methyl Acetate	2.99	43	3806	4.78	ppb	89
22) Iodomethane	2.66	142	7587	5.42	ppb	98
23) Acrylonitrile	3.43	53	2612	5.94	ppb	91
25) Methylene chloride	3.08	84	8233	5.04	ppb	88
26) Carbon disulfide	2.72	76	10258	4.71	ppb	98
27) Methyl t-butyl ether (MtBE	3.47	73	28794	5.49	ppb	96
28) Trans-1,2-DCE	3.43	96	9294	5.40	ppb	89
29) 3-Methylpentane	3.46	57	5115	5.47	ppb	91
30) Hexane	3.72	56	213	10.02	ppb	# 100

(#) = qualifier out of range (m) = manual integration
 1015M16.D M1015W.M Wed Oct 20 12:06:37 2021

Data File : M:\MAX\DATA\211015\1015M16.D
 Acq On : 15 Oct 21 17:06
 Sample : 5ug/L VOC STD 10/15/21
 Misc : IS&S 8/4/21

Vial: 6
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 13:28:38 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
31) Diisopropyl Ether	4.25	45	19726	5.43	ppb	92
32) 1,1-DCA	4.05	63	14219	5.28	ppb #	85
33) Vinyl Acetate	4.16	43	159	0.12	ppb #	77
34) Ethyl tert Butyl Ether	4.77	59	24023	5.05	ppb	89
35) Methylcyclopentane	4.77	56	1134	5.67	ppb	100
36) MEK (2-Butanone)	4.99	43	20148	39.03	ppb	88
37) Cis-1,2-DCE	4.91	96	10198	5.44	ppb	96
38) 2,2-Dichloropropane	4.89	77	17894	5.13	ppb	98
39) Chloroform	5.37	83	19904	5.41	ppb	99
40) Bromochloromethane	5.22	130	8478	5.52	ppb #	83
42) 1,1,1-TCA	5.54	97	22632	5.88	ppb	93
43) Cyclohexane	5.58	41	6390	5.53	ppb	76
44) 1,1-Dichloropropene	5.75	75	12969	5.98	ppb	85
45) 2,2,4-Trimethylpentane	6.11	57	14248	4.15	ppb	87
47) Carbon Tetrachloride	5.73	117	21221	6.09	ppb	90
48) Tert Amyl Methyl Ether	6.18	73	23576	5.01	ppb	98
49) 1,2-DCA	6.04	62	18340	5.49	ppb	98
50) Benzene	5.99	78	33663	5.51	ppb	98
51) TCE	6.75	95	9650	4.55	ppb #	77
52) 2-Pentanone	7.01	43	86889	101.33	ppb	97
53) 1,2-Dichloropropane	7.00	63	3245	4.78	ppb #	92
54) Bromodichloromethane	7.31	83	17085	5.99	ppb	90
55) Methyl Cyclohexane	6.94	83	11773	4.68	ppb	91
56) Dibromomethane	7.12	93	6546	5.99	ppb	88
57) MIBK (methyl isobutyl ket	7.98	43	43474	37.27	ppb	98
58) 1-Bromo-2-chloroethane	7.62	144	2479	6.12	ppb	78
59) 2-Chloroethyl vinyl ether	7.61	43	20	16.23	ppb #	100
60) Cis-1,3-Dichloropropene	7.79	75	14773	5.52	ppb	90
61) Toluene	8.12	91	39874	5.31	ppb	96
62) Trans-1,3-Dichloropropene	8.37	75	14624	5.33	ppb	99
63) 1,1,2-TCA	8.55	83	5668	4.81	ppb	89
64) 2-Hexanone	8.83	43	28901	34.73	ppb #	97
67) 1,2-EDB	9.03	107	9212	5.97	ppb	93
68) Tetrachloroethene	8.66	164	9368	6.20	ppb	96
69) 1-Chlorohexane	9.53	91	7028	5.15	ppb	83
70) 1,1,1,2-Tetrachloroethane	9.62	131	14631	5.77	ppb	92
71) m&p-Xylene	9.77	106	40521	10.70	ppb	97
72) o-Xylene	10.16	106	19748	5.15	ppb	89
73) Styrene	10.18	104	31878	5.09	ppb	98
75) 1,3-Dichloropropane	8.71	76	13752	5.80	ppb	98
76) Dibromochloromethane	8.93	129	13298	5.58	ppb	89
77) Chlorobenzene	9.53	112	30958	5.33	ppb	96

(#) = qualifier out of range (m) = manual integration

Data File : M:\MAX\DATA\211015\1015M16.D
 Acq On : 15 Oct 21 17:06
 Sample : 5ug/L VOC STD 10/15/21
 Misc : IS&S 8/4/21

Vial: 6
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 13:28:38 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
78) Ethylbenzene	9.65	91	49016	5.60	ppb	98
79) Bromoform	10.35	173	10773	5.43	ppb	98
81) Isopropylbenzene	10.53	105	53902	5.30	ppb	98
82) 1,1,2,2-Tetrachloroethane	10.84	83	8866	5.20	ppb	# 85
83) 1,2,3-Trichloropropane	10.88	110	4864	5.78	ppb	# 73
84) t-1,4-Dichloro-2-Butene	10.91	53	2090	4.29	ppb	84
85) Bromobenzene	10.81	156	17611	5.08	ppb	88
86) n-Propylbenzene	10.94	91	52829	5.19	ppb	95
87) 4-Ethyltoluene	11.06	105	48078	5.06	ppb	92
88) 2-Chlorotoluene	11.01	91	41952	5.29	ppb	89
89) 1,3,5-Trimethylbenzene	11.12	105	46678	5.36	ppb	97
90) 4-Chlorotoluene	11.13	91	41644	5.22	ppb	99
91) Tert-Butylbenzene	11.44	119	26648	5.40	ppb	93
92) 1,2,4-Trimethylbenzene	11.49	105	45050	5.34	ppb	99
93) Sec-Butylbenzene	11.66	105	49880	5.44	ppb	98
94) p-Isopropyltoluene	11.81	119	48782	5.36	ppb	99
95) Benzyl Chloride	11.99	91	10073	4.36	ppb	# 96
96) 1,3-DCB	11.75	146	31609	5.56	ppb	95
97) 1,4-DCB	11.85	146	29696	4.96	ppb	95
98) n-Butylbenzene	12.22	91	26294	4.95	ppb	97
99) 1,2-DCB	12.21	146	30601	5.46	ppb	87
100) Hexachloroethane	12.46	117	7449	4.82	ppb	86
101) 1,2-Dibromo-3-chloropropan	12.99	75	2238	5.40	ppb	84
102) 1,2,4-Trichlorobenzene	13.81	180	7399	4.97	ppb	85
103) Hexachlorobutadiene	13.99	225	10435	4.84	ppb	92
104) Naphthalene	14.06	128	14154	4.85	ppb	95
105) 1,2,3-Trichlorobenzene	14.29	180	9443	5.76	ppb	82

Quantitation Report


Data File : M:\MAX\DATA\211015\1015M16.D
Acq On : 15 Oct 21 17:06
Sample : 5ug/L VOC STD 10/15/21
Misc : IS&S 8/4/21

Vial: 6
Operator: LP,DG,CH
Inst : Max
Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
Title : METHOD 8260B
Last Update : Sat Oct 16 14:01:48 2021
Response via : Initial Calibration

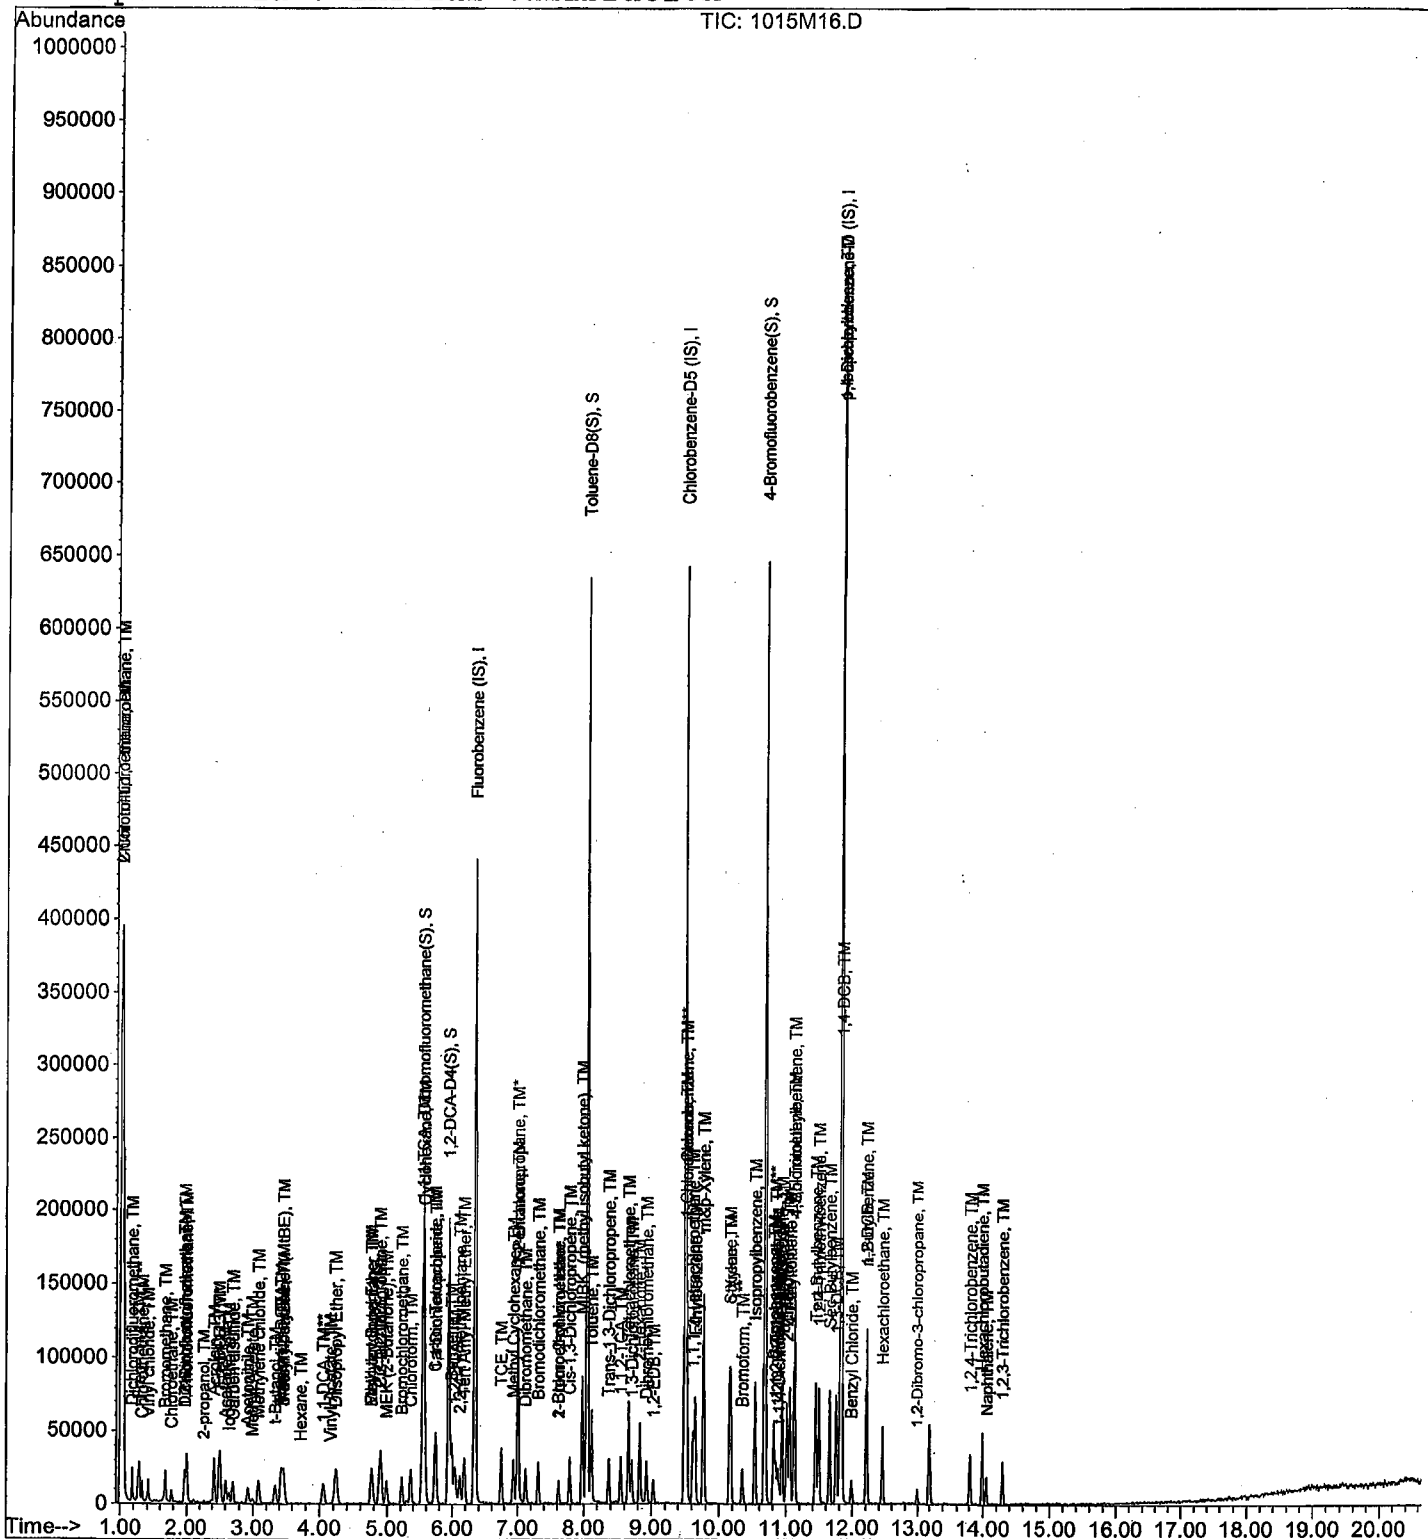

Data File : M:\MAX\DATA\211015\1015M17.D
 Acq On : 15 Oct 21 17:35
 Sample : 10ug/L VOC STD 10/15/21
 Misc : IS&S 8/4/21

Vial: 7
 Operator: LP, DG, CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 13:28:38 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.34	96	377347	25.00	ppb	0.00
65) Chlorobenzene-D5 (IS)	9.50	117	347072	25.00	ppb	0.00
80) 1,4-Dichlorobenzene-D (IS)	11.82	152	236441	25.00	ppb	0.00

System Monitoring Compounds

41) Dibromofluoromethane(S)	5.56	111	118319	25.95	ppb	0.00	
Spiked Amount				25.000			Recovery = 103.780%
46) 1,2-DCA-D4(S)	5.95	65	79312	25.60	ppb	0.00	
Spiked Amount				25.000			Recovery = 102.392%
66) Toluene-D8(S)	8.05	98	392721	25.00	ppb	0.00	
Spiked Amount				25.000			Recovery = 99.988%
74) 4-Bromofluorobenzene(S)	10.68	95	160324	23.71	ppb	0.00	
Spiked Amount				25.000			Recovery = 94.848%

Target Compounds

	R.T.	QIon	Response	Conc	Units	Qvalue
2) Chlorotrifluoroethene	1.01	116	1480	10.00	ppb	100
3) Dichlorodifluoromethane	1.19	85	19568	10.22	ppb	100
4) Freon 114	1.29	85	10651	6.61	ppb	100
5) Chloromethane	1.33	50	13364	11.30	ppb	100
6) Vinyl chloride	1.42	62	16573	11.82	ppb	100
7) 2-Chloro-1,1,1-trifluoroet	1.01	118	2056	50.00	ppb	100
8) Bromomethane	1.68	94	12882	13.34	ppb	100
9) Chloroethane	1.77	64	11250	11.78	ppb	100
10) Dichlorofluoromethane	1.97	67	36430	11.39	ppb	100
11) Trichlorofluoromethane	2.00	101	43493	12.08	ppb	100
12) 2,2-Dichloro-1,1,1-trifluo	2.29	85	23	20.00	ppb	100
13) Acrolein	2.43	56	26701	75.38	ppb	100
14) Acetone	2.61	43	24111	56.01	ppb	100
15) Freon-113	2.53	151	16125	9.66	ppb	100
16) Acetonitrile	2.92	41	13763	114.30	ppb	100
17) 2-propanol	2.26	45	892	50.00	ppb	100
18) 1,2-Dichlorotrifluoroethan	1.97	67	36430	11.39	ppb	100
19) 1,1-DCE	2.51	61	25329	11.55	ppb	100
20) t-Butanol	3.34	59	19181	118.01	ppb	100
21) Methyl Acetate	3.00	43	8263	10.66	ppb	100
22) Iodomethane	2.66	142	17486	11.16	ppb	100
23) Acrylonitrile	3.43	53	4844	11.24	ppb	100
24) 2-Methylpentane	2.16	71	23	10.00	ppb	100
25) Methylene chloride	3.08	84	17432	10.96	ppb	100
26) Carbon disulfide	2.71	76	20960	9.87	ppb	100
27) Methyl t-butyl ether (MtBE)	3.47	73	57116	11.18	ppb	100
28) Trans-1,2-DCE	3.43	96	17741	11.38	ppb	100

Data File : M:\MAX\DATA\211015\1015M17.D
 Acq On : 15 Oct 21 17:35
 Sample : 10ug/L VOC STD 10/15/21
 Misc : IS&S 8/4/21

Vial: 7
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 13:28:38 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
29) 3-Methylpentane	3.46	57	10024	11.67	ppb	100
30) Hexane	3.72	56	414	20.00	ppb	100
31) Diisopropyl Ether	4.24	45	37208	10.51	ppb	100
32) 1,1-DCA	4.05	63	28067	10.71	ppb	100
34) Ethyl tert Butyl Ether	4.77	59	46096	9.95	ppb	100
35) Methylcyclopentane	4.77	56	1948	10.00	ppb	100
36) MEK (2-Butanone)	4.99	43	26957	53.62	ppb	100
37) Cis-1,2-DCE	4.91	96	20531	11.24	ppb	100
38) 2,2-Dichloropropane	4.89	77	37047	10.91	ppb	100
39) Chloroform	5.36	83	41151	11.48	ppb	100
40) Bromochloromethane	5.22	130	15934	11.39	ppb	100
42) 1,1,1-TCA	5.55	97	43737	11.67	ppb	100
43) Cyclohexane	5.58	41	10585	9.41	ppb	100
44) 1,1-Dichloropropene	5.75	75	23149	10.97	ppb	100
45) 2,2,4-Trimethylpentane	6.12	57	25327	7.58	ppb	100
47) Carbon Tetrachloride	5.73	117	40318	11.88	ppb	100
48) Tert Amyl Methyl Ether	6.18	73	47074	10.27	ppb	100
49) 1,2-DCA	6.04	62	36487	11.21	ppb	100
50) Benzene	5.99	78	67135	11.28	ppb	100
51) TCE	6.75	95	21853	11.75	ppb	100
52) 2-Pentanone	7.01	43	108759	130.21	ppb	100
53) 1,2-Dichloropropane	7.00	63	7561	11.89	ppb	100
54) Bromodichloromethane	7.31	83	30571	11.00	ppb	100
55) Methyl Cyclohexane	6.94	83	20502	8.86	ppb	100
56) Dibromomethane	7.12	93	12823	12.05	ppb	100
57) MIBK (methyl isobutyl ket	7.98	43	56842	50.03	ppb	100
58) 1-Bromo-2-chloroethane	7.62	144	4063	10.30	ppb	100
59) 2-Chloroethyl vinyl ether	7.67	43	72	60.00	ppb	# 100
60) Cis-1,3-Dichloropropene	7.79	75	27754	10.65	ppb	100
61) Toluene	8.12	91	82436	11.27	ppb	100
62) Trans-1,3-Dichloropropene	8.37	75	28083	10.50	ppb	100
63) 1,1,2-TCA	8.55	83	12220	10.64	ppb	100
64) 2-Hexanone	8.83	43	39749	49.04	ppb	100
67) 1,2-EDB	9.03	107	17939	11.55	ppb	100
68) Tetrachloroethene	8.66	164	16284	10.70	ppb	100
69) 1-Chlorohexane	9.53	91	12452	9.07	ppb	100
70) 1,1,1,2-Tetrachloroethane	9.62	131	28021	10.98	ppb	100
71) m&p-Xylene	9.77	106	82514	21.66	ppb	100
72) o-Xylene	10.16	106	40678	10.54	ppb	100
73) Styrene	10.18	104	66045	10.48	ppb	100
75) 1,3-Dichloropropane	8.71	76	26720	11.19	ppb	100
76) Dibromochloromethane	8.93	129	26700	11.13	ppb	100

(#) = qualifier out of range (m) = manual integration
 1015M17.D M1015W.M Wed Oct 20 12:06:39 2021

Data File : M:\MAX\DATA\211015\1015M17.D
 Acq On : 15 Oct 21 17:35
 Sample : 10ug/L VOC STD 10/15/21
 Misc : IS&S 8/4/21

Vial: 7
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 13:28:38 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
77) Chlorobenzene	9.53	112	61648	10.55	ppb	100
78) Ethylbenzene	9.65	91	94727	10.75	ppb	100
79) Bromoform	10.35	173	22290	11.17	ppb	100
81) Isopropylbenzene	10.53	105	106456	10.30	ppb	100
82) 1,1,2,2-Tetrachloroethane	10.84	83	18342	10.58	ppb	100
83) 1,2,3-Trichloropropane	10.87	110	9043	10.87	ppb	100
84) t-1,4-Dichloro-2-Butene	10.90	53	4578	8.87	ppb	100
85) Bromobenzene	10.81	156	34140	9.67	ppb	100
86) n-Propylbenzene	10.94	91	111438	10.76	ppb	100
87) 4-Ethyltoluene	11.06	105	102117	10.56	ppb	100
88) 2-Chlorotoluene	11.01	91	87062	10.80	ppb	100
89) 1,3,5-Trimethylbenzene	11.12	105	98343	11.10	ppb	100
90) 4-Chlorotoluene	11.13	91	85815	10.58	ppb	100
91) Tert-Butylbenzene	11.44	119	53976	10.76	ppb	100
92) 1,2,4-Trimethylbenzene	11.49	105	92332	10.53	ppb	100
93) Sec-Butylbenzene	11.66	105	104508	11.21	ppb	100
94) p-Isopropyltoluene	11.81	119	100003	10.46	ppb	100
95) Benzyl Chloride	11.99	91	20556	8.75	ppb	100
96) 1,3-DCB	11.75	146	62186	10.76	ppb	100
97) 1,4-DCB	11.84	146	61854	10.71	ppb	100
98) n-Butylbenzene	12.22	91	56499	9.46	ppb	100
99) 1,2-DCB	12.21	146	61844	10.85	ppb	100
100) Hexachloroethane	12.46	117	14896	9.62	ppb	100
101) 1,2-Dibromo-3-chloropropan	12.99	75	5285	11.44	ppb	100
102) 1,2,4-Trichlorobenzene	13.81	180	18752	9.24	ppb	100
103) Hexachlorobutadiene	13.99	225	23952	9.95	ppb	100
104) Naphthalene	14.05	128	39199	11.87	ppb	100
105) 1,2,3-Trichlorobenzene	14.30	180	23602	9.93	ppb	100

Quantitation Report


Data File : M:\MAX\DATA\211015\1015M17.D
 Acq On : 15 Oct 21 17:35
 Sample : 10ug/L VOC STD 10/15/21
 Misc : IS&S 8/4/21

Vial: 7
 Operator: LP, DG, CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 14:01:48 2021
 Response via : Initial Calibration

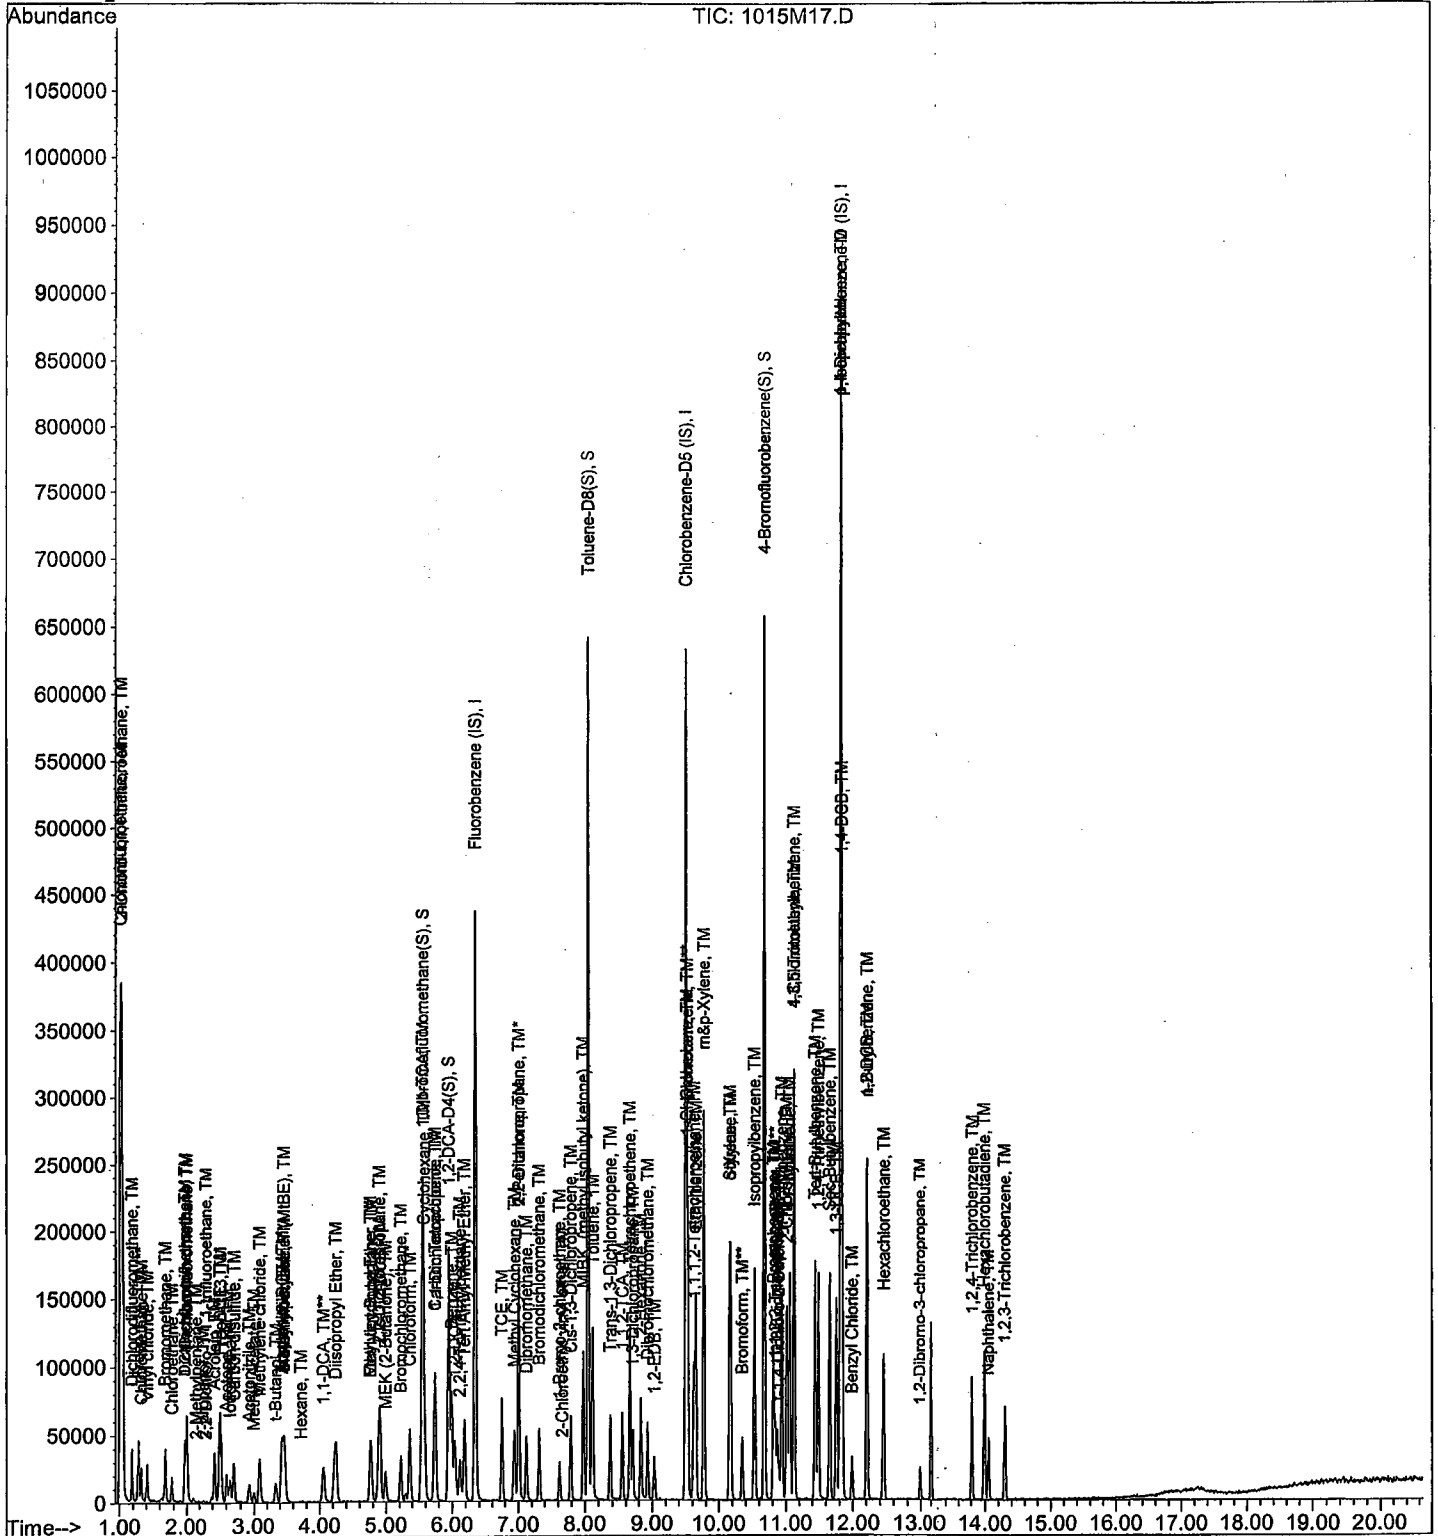

Data File : M:\MAX\DATA\211015\1015M18.D
 Acq On : 15 Oct 21 18:03
 Sample : 20ug/L VOC STD 10/15/21
 Misc : IS&S 8/4/21

Vial: 8
 Operator: LP, DG, CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 13:28:38 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.34	96	395871	25.00	ppb	0.00
65) Chlorobenzene-D5 (IS)	9.50	117	351611	25.00	ppb	0.00
80) 1,4-Dichlorobenzene-D (IS)	11.82	152	235162	25.00	ppb	0.00
System Monitoring Compounds						
41) Dibromofluoromethane (S)	5.56	111	236514	49.44	ppb	0.00
Spiked Amount	25.000		Recovery	=	197.748%	
46) 1,2-DCA-D4 (S)	5.95	65	166400	51.19	ppb	0.00
Spiked Amount	25.000		Recovery	=	204.772%	
66) Toluene-D8 (S)	8.05	98	780890	49.06	ppb	0.00
Spiked Amount	25.000		Recovery	=	196.252%	
74) 4-Bromofluorobenzene (S)	10.68	95	327466	47.81	ppb	0.00
Spiked Amount	25.000		Recovery	=	191.232%	
Target Compounds						
2) Chlorotrifluoroethene	1.03	116	1543	9.94	ppb #	60
3) Dichlorodifluoromethane	1.18	85	43432	21.62	ppb	97
4) Freon 114	1.29	85	29061	17.19	ppb	81
5) Chloromethane	1.33	50	25172	20.46	ppb	98
6) Vinyl chloride	1.42	62	33428	22.72	ppb	95
7) 2-Chloro-1,1,1-trifluoroet	1.00	118	1142	26.47	ppb #	37
8) Bromomethane	1.68	94	25141	25.37	ppb	95
9) Chloroethane	1.77	64	20310	20.33	ppb	99
10) Dichlorofluoromethane	1.97	67	69254	20.65	ppb	99
11) Trichlorofluoromethane	2.00	101	90422	23.94	ppb	91
12) 2,2-Dichloro-1,1,1-trifluo	2.27	85	19	15.75	ppb	100
13) Acrolein	2.44	56	32051	86.25	ppb	99
14) Acetone	2.61	43	29127	64.50	ppb	99
15) Freon-113	2.53	151	37209	21.25	ppb	94
16) Acetonitrile	2.93	41	18046	142.86	ppb	93
17) 2-propanol	2.26	45	2021	107.98	ppb #	81
18) 1,2-Dichlorotrifluoroethan	1.97	67	69254	20.64	ppb	100
19) 1,1-DCE	2.51	61	53746	23.36	ppb	97
20) t-Butanol	3.34	59	23282	129.99	ppb	92
21) Methyl Acetate	2.99	43	16974	20.87	ppb	100
22) Iodomethane	2.66	142	35780	20.61	ppb	93
23) Acrylonitrile	3.43	53	10005	22.05	ppb #	84
24) 2-Methylpentane	2.10	71	44	18.24	ppb #	100
25) Methylene chloride	3.08	84	34285	20.55	ppb	94
26) Carbon disulfide	2.71	76	44096	19.79	ppb	97
27) Methyl t-butyl ether (MtBE	3.47	73	114470	21.36	ppb	100
28) Trans-1,2-DCE	3.43	96	38698	24.57	ppb	94

(#) = qualifier out of range (m) = manual integration
 1015M18.D M1015W.M Wed Oct 20 12:06:41 2021

Data File : M:\MAX\DATA\211015\1015M18.D
 Acq On : 15 Oct 21 18:03
 Sample : 20ug/L VOC STD 10/15/21
 Misc : IS&S 8/4/21

Vial: 8
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 13:28:38 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
29) 3-Methylpentane	3.47	57	21607	24.67	ppb	96
30) Hexane	3.73	56	771	35.50	ppb	100
31) Diisopropyl Ether	4.24	45	74704	20.11	ppb	96
32) 1,1-DCA	4.06	63	59120	21.50	ppb	98
34) Ethyl tert Butyl Ether	4.77	59	95539	19.66	ppb	95
35) Methylcyclopentane	4.77	56	3929	19.23	ppb	# 100
36) MEK (2-Butanone)	4.99	43	30811	58.42	ppb	# 91
37) Cis-1,2-DCE	4.91	96	40102	20.93	ppb	94
38) 2,2-Dichloropropane	4.89	77	73086	20.52	ppb	99
39) Chloroform	5.36	83	81653	21.71	ppb	100
40) Bromochloromethane	5.22	130	33221	23.42	ppb	93
42) 1,1,1-TCA	5.54	97	93844	23.87	ppb	95
43) Cyclohexane	5.58	41	24494	20.75	ppb	85
44) 1,1-Dichloropropene	5.75	75	49132	22.19	ppb	93
45) 2,2,4-Trimethylpentane	6.12	57	57952	16.53	ppb	# 81
47) Carbon Tetrachloride	5.73	117	81738	22.96	ppb	94
48) Tert Amyl Methyl Ether	6.18	73	93531	19.46	ppb	97
49) 1,2-DCA	6.04	62	73123	21.42	ppb	97
50) Benzene	5.99	78	134429	21.52	ppb	95
51) TCE	6.75	95	41884	22.20	ppb	85
52) 2-Pentanone	7.01	43	131778	150.39	ppb	97
53) 1,2-Dichloropropane	7.00	63	15331	23.28	ppb	99
54) Bromodichloromethane	7.31	83	63530	21.79	ppb	94
55) Methyl Cyclohexane	6.94	83	47883	20.50	ppb	99
56) Dibromomethane	7.12	93	24263	21.72	ppb	99
57) MIBK (methyl isobutyl ket	7.98	43	66896	56.12	ppb	96
58) 1-Bromo-2-chloroethane	7.62	144	8668	20.95	ppb	82
59) 2-Chloroethyl vinyl ether	7.64	43	135	107.24	ppb	# 100
60) Cis-1,3-Dichloropropene	7.79	75	58299	21.33	ppb	92
61) Toluene	8.12	91	158484	20.66	ppb	98
62) Trans-1,3-Dichloropropene	8.37	75	58054	20.70	ppb	99
63) 1,1,2-TCA	8.55	83	23159	19.22	ppb	98
64) 2-Hexanone	8.83	43	48162	56.64	ppb	96
67) 1,2-EDB	9.03	107	37727	23.98	ppb	91
68) Tetrachloroethene	8.66	164	37992	24.65	ppb	# 77
69) 1-Chlorohexane	9.53	91	27928	20.08	ppb	92
70) 1,1,1,2-Tetrachloroethane	9.62	131	54825	21.21	ppb	97
71) m&p-Xylene	9.77	106	168462	43.65	ppb	94
72) o-Xylene	10.16	106	80768	20.66	ppb	96
73) Styrene	10.18	104	132105	20.70	ppb	100
75) 1,3-Dichloropropane	8.71	76	51570	21.33	ppb	# 81
76) Dibromochloromethane	8.93	129	55342	22.78	ppb	97

(#) = qualifier out of range (m) = manual integration

Data File : M:\MAX\DATA\211015\1015M18.D
 Acq On : 15 Oct 21 18:03
 Sample : 20ug/L VOC STD 10/15/21
 Misc : IS&S 8/4/21

Vial: 8
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 13:28:38 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
77) Chlorobenzene	9.53	112	123674	20.90	ppb	95
78) Ethylbenzene	9.65	91	190505	21.35	ppb	99
79) Bromoform	10.35	173	46086	22.80	ppb	91
81) Isopropylbenzene	10.53	105	215921	21.00	ppb	96
82) 1,1,2,2-Tetrachloroethane	10.84	83	34580	20.06	ppb	93
83) 1,2,3-Trichloropropane	10.88	110	18655	22.95	ppb	93
84) t-1,4-Dichloro-2-Butene	10.90	53	9193	17.59	ppb	76
85) Bromobenzene	10.81	156	72807	20.74	ppb	87
86) n-Propylbenzene	10.94	91	218212	21.18	ppb	98
87) 4-Ethyltoluene	11.06	105	204272	21.24	ppb	94
88) 2-Chlorotoluene	11.01	91	166317	20.74	ppb	92
89) 1,3,5-Trimethylbenzene	11.12	105	188460	21.39	ppb	96
90) 4-Chlorotoluene	11.13	91	169578	21.02	ppb	99
91) Tert-Butylbenzene	11.44	119	113528	22.75	ppb	98
92) 1,2,4-Trimethylbenzene	11.49	105	194704	22.09	ppb	97
93) Sec-Butylbenzene	11.66	105	210964	22.75	ppb	99
94) p-Isopropyltoluene	11.81	119	210376	21.74	ppb	98
95) Benzyl Chloride	11.99	91	42029	17.98	ppb	97
96) 1,3-DCB	11.75	146	126212	21.95	ppb	98
97) 1,4-DCB	11.84	146	125705	22.43	ppb	96
98) n-Butylbenzene	12.22	91	128982	20.53	ppb	95
99) 1,2-DCB	12.21	146	124816	22.02	ppb	98
100) Hexachloroethane	12.46	117	30628	20.04	ppb	94
101) 1,2-Dibromo-3-chloropropan	12.99	75	10893	22.83	ppb	# 81
102) 1,2,4-Trichlorobenzene	13.81	180	49784	21.15	ppb	88
103) Hexachlorobutadiene	13.99	225	53060	21.20	ppb	97
104) Naphthalene	14.05	128	96821	26.22	ppb	99
105) 1,2,3-Trichlorobenzene	14.30	180	62906	21.74	ppb	86

Quantitation Report


Data File : M:\MAX\DATA\211015\1015M18.D
Acq On : 15 Oct 21 18:03
Sample : 20ug/L VOC STD 10/15/21
Misc : IS&S 8/4/21

Vial: 8
Operator: LP, DG, CH
Inst : Max
Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
Title : METHOD 8260B
Last Update : Sat Oct 16 14:01:48 2021
Response via : Initial Calibration

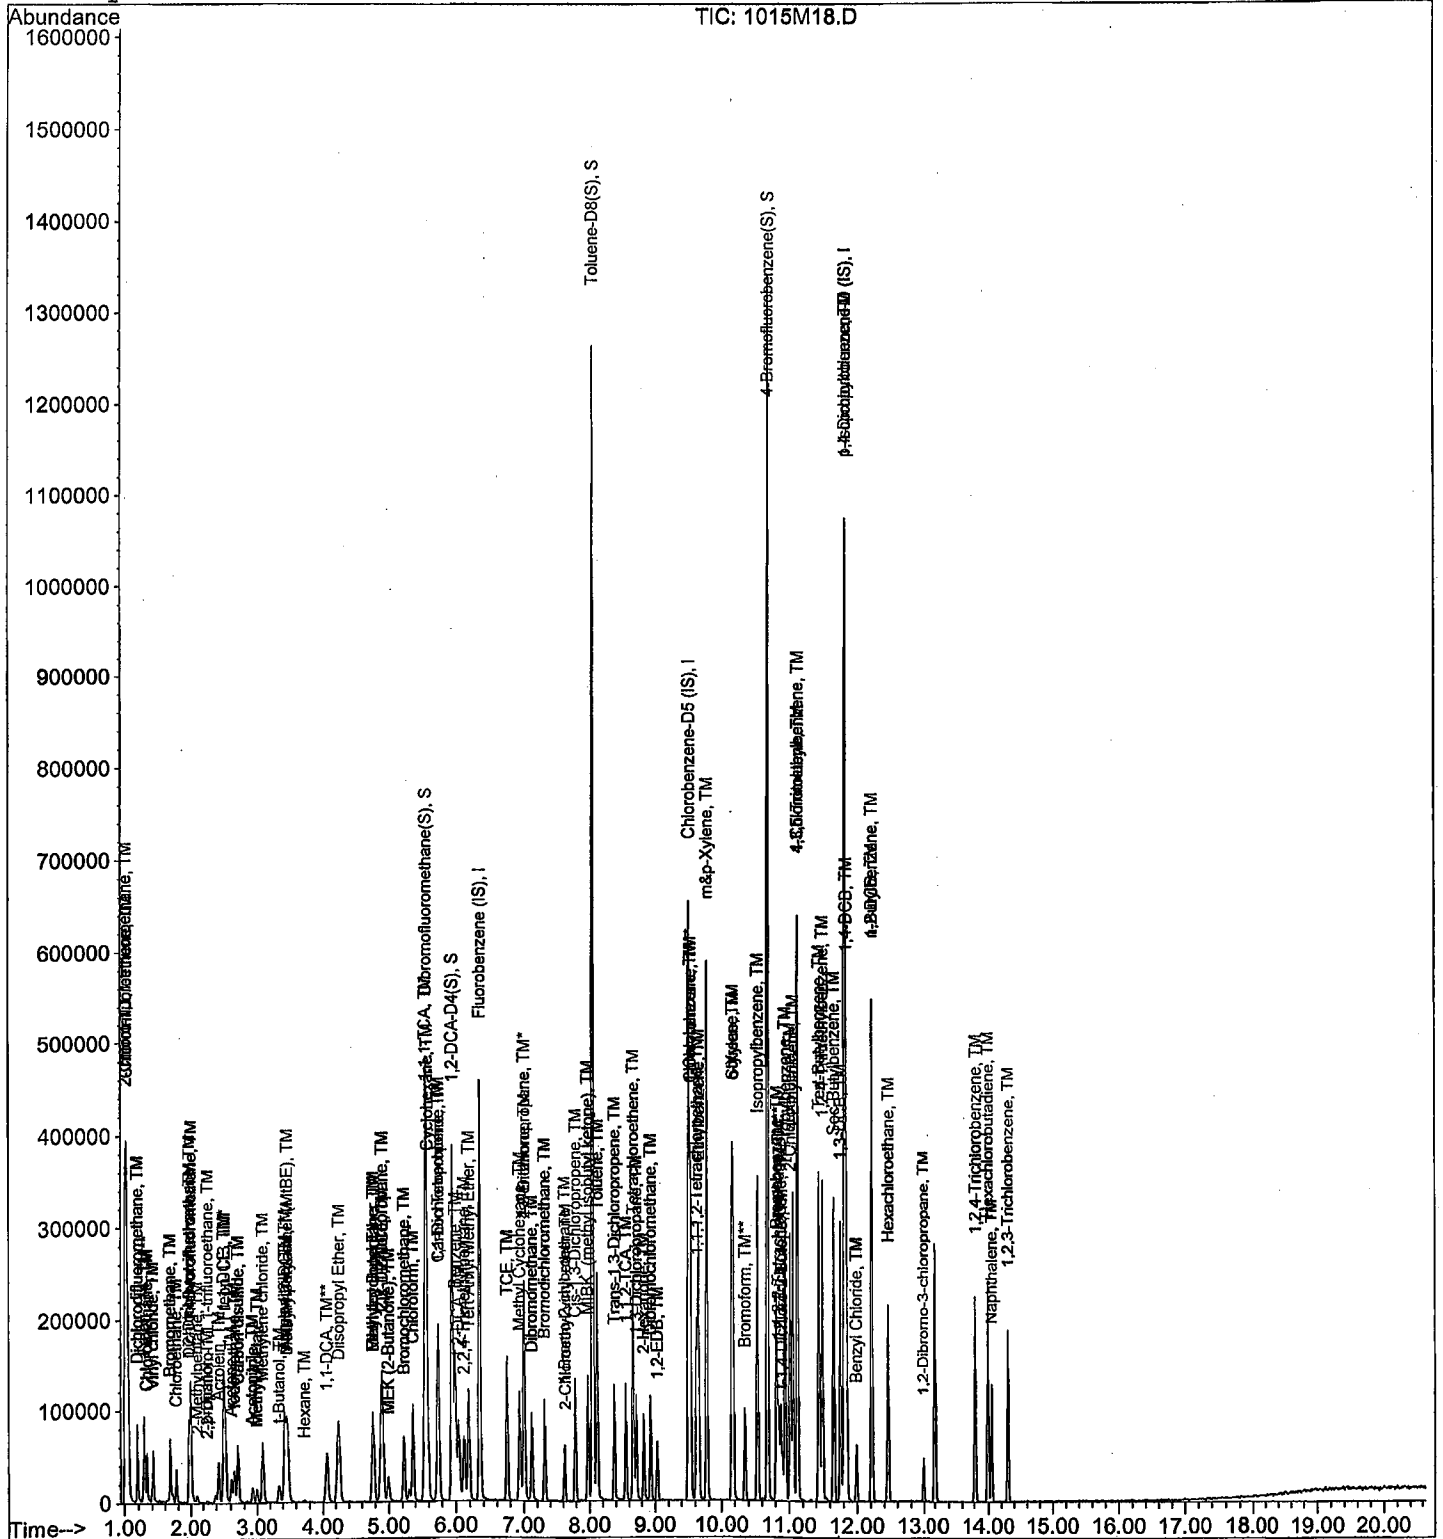

Data File : M:\MAX\DATA\211015\1015M19.D
 Acq On : 15 Oct 21 18:31
 Sample : 40ug/L VOC STD 10/15/21
 Misc : IS&S 8/4/21

Vial: 9
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 13:28:38 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.34	96	394795	25.00	ppb	0.00
65) Chlorobenzene-D5 (IS)	9.50	117	356570	25.00	ppb	0.00
80) 1,4-Dichlorobenzene-D (IS)	11.82	152	246902	25.00	ppb	0.00
System Monitoring Compounds						
41) Dibromofluoromethane (S)	5.56	111	238087	49.90	ppb	0.00
Spiked Amount						
Recovery						= 199.604%
46) 1,2-DCA-D4 (S)	5.95	65	166336	51.31	ppb	0.00
Spiked Amount						
Recovery						= 205.252%
66) Toluene-D8 (S)	8.05	98	788816	48.87	ppb	0.00
Spiked Amount						
Recovery						= 195.484%
74) 4-Bromofluorobenzene (S)	10.68	95	335059	48.24	ppb	0.00
Spiked Amount						
Recovery						= 192.944%
Target Compounds						
2) Chlorotrifluoroethene	1.01	116	1951	12.60	ppb	# 73
3) Dichlorodifluoromethane	1.18	85	95360	47.61	ppb	100
4) Freon 114	1.29	85	57360	34.02	ppb	83
5) Chloromethane	1.33	50	56542	46.36	ppb	94
6) Vinyl chloride	1.42	62	70630	48.13	ppb	92
7) 2-Chloro-1,1,1-trifluoroet	1.01	118	1922	44.68	ppb	# 51
8) Bromomethane	1.68	94	51410	52.69	ppb	91
9) Chloroethane	1.77	64	42072	42.31	ppb	97
10) Dichlorofluoromethane	1.97	67	141160	42.20	ppb	99
11) Trichlorofluoromethane	2.00	101	187948	49.90	ppb	98
12) 2,2-Dichloro-1,1,1-trifluo	2.18	85	25	20.78	ppb	100
13) Acrolein	2.43	56	40051	108.07	ppb	88
14) Acetone	2.62	43	39041	86.69	ppb	98
15) Freon-113	2.52	151	70973	40.64	ppb	97
16) Acetonitrile	2.93	41	22065	175.15	ppb	88
17) 2-propanol	2.27	45	3181	170.43	ppb	# 81
18) 1,2-Dichlorotrifluoroethan	1.97	67	141160	42.19	ppb	100
19) 1,1-DCE	2.50	61	104417	45.50	ppb	96
20) t-Butanol	3.35	59	36678	173.72	ppb	96
21) Methyl Acetate	2.99	43	34963	43.11	ppb	95
22) Iodomethane	2.66	142	81874	45.72	ppb	95
23) Acrylonitrile	3.43	53	19528	43.06	ppb	# 80
24) 2-Methylpentane	2.10	71	116	48.21	ppb	# 100
25) Methylene chloride	3.08	84	68587	41.23	ppb	97
26) Carbon disulfide	2.71	76	86056	38.73	ppb	99
27) Methyl t-butyl ether (MtBE	3.47	73	239816	44.88	ppb	94
28) Trans-1,2-DCE	3.43	96	72205	46.70	ppb	95

(#) = qualifier out of range (m) = manual integration
 1015M19.D M1015W.M Wed Oct 20 12:06:43 2021

Data File : M:\MAX\DATA\211015\1015M19.D
 Acq On : 15 Oct 21 18:31
 Sample : 40ug/L VOC STD 10/15/21
 Misc : IS&S 8/4/21

Vial: 9
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 13:28:38 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
29) 3-Methylpentane	3.47	57	37452	43.35	ppb	88
30) Hexane	3.70	56	751	34.68	ppb #	100
31) Diisopropyl Ether	4.24	45	152386	41.14	ppb	95
32) 1,1-DCA	4.06	63	116415	42.45	ppb #	94
34) Ethyl tert Butyl Ether	4.77	59	199919	41.25	ppb	94
35) Methylcyclopentane	4.77	56	8348	40.96	ppb	100
36) MEK (2-Butanone)	4.99	43	43256	82.23	ppb	88
37) Cis-1,2-DCE	4.91	96	82880	43.37	ppb	92
38) 2,2-Dichloropropane	4.89	77	141607	39.86	ppb	99
39) Chloroform	5.36	83	160419	42.76	ppb	94
40) Bromochloromethane	5.22	130	68479	49.26	ppb	94
42) 1,1,1-TCA	5.54	97	182393	46.52	ppb	98
43) Cyclohexane	5.58	41	48312	41.04	ppb	90
44) 1,1-Dichloropropene	5.75	75	94511	42.80	ppb	97
45) 2,2,4-Trimethylpentane	6.12	57	121452	34.73	ppb #	86
47) Carbon Tetrachloride	5.74	117	166925	47.02	ppb	98
48) Tert Amyl Methyl Ether	6.18	73	194157	40.51	ppb	97
49) 1,2-DCA	6.04	62	153949	45.21	ppb	100
50) Benzene	5.99	78	269561	43.28	ppb	99
51) TCE	6.75	95	85080	46.13	ppb	85
52) 2-Pentanone	7.01	43	159478	182.50	ppb	99
53) 1,2-Dichloropropane	7.00	63	32440	49.75	ppb	96
54) Bromodichloromethane	7.31	83	132884	45.71	ppb	99
55) Methyl Cyclohexane	6.94	83	97260	42.40	ppb	100
56) Dibromomethane	7.12	93	50236	45.10	ppb	93
57) MIBK (methyl isobutyl ket	7.98	43	93060	78.28	ppb	97
58) 1-Bromo-2-chloroethane	7.62	144	17760	43.04	ppb	98
59) 2-Chloroethyl vinyl ether	7.58	43	20	15.93	ppb #	100
60) Cis-1,3-Dichloropropene	7.79	75	117498	43.10	ppb	96
61) Toluene	8.12	91	319786	41.80	ppb	99
62) Trans-1,3-Dichloropropene	8.37	75	122778	43.89	ppb	99
63) 1,1,2-TCA	8.55	83	47558	39.57	ppb	94
64) 2-Hexanone	8.83	43	66653	78.60	ppb	94
67) 1,2-EDB	9.03	107	74115	46.45	ppb	95
68) Tetrachloroethene	8.66	164	70304	44.97	ppb	81
69) 1-Chlorohexane	9.53	91	54312	38.51	ppb	96
70) 1,1,1,2-Tetrachloroethane	9.62	131	111805	42.65	ppb	92
71) m&p-Xylene	9.77	106	333019	85.09	ppb	100
72) o-Xylene	10.16	106	167690	42.31	ppb	100
73) Styrene	10.18	104	270125	41.74	ppb	99
75) 1,3-Dichloropropane	8.71	76	106532	43.44	ppb	88
76) Dibromochloromethane	8.93	129	113393	46.02	ppb	99

(#) = qualifier out of range (m) = manual integration
 1015M19.D M1015W.M Wed Oct 20 12:06:43 2021

Data File : M:\MAX\DATA\211015\1015M19.D
 Acq On : 15 Oct 21 18:31
 Sample : 40ug/L VOC STD 10/15/21
 Misc : IS&S 8/4/21

Vial: 9
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 13:28:38 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
77) Chlorobenzene	9.53	112	247111	41.17	ppb	96
78) Ethylbenzene	9.65	91	393606	43.49	ppb	98
79) Bromoform	10.35	173	96934	47.29	ppb	94
81) Isopropylbenzene	10.53	105	436071	40.40	ppb	98
82) 1,1,2,2-Tetrachloroethane	10.84	83	72110	39.85	ppb	91
83) 1,2,3-Trichloropropane	10.88	110	37233	43.97	ppb	94
84) t-1,4-Dichloro-2-Butene	10.90	53	20351	36.72	ppb	74
85) Bromobenzene	10.81	156	144680	39.26	ppb	93
86) n-Propylbenzene	10.94	91	452586	41.83	ppb	99
87) 4-Ethyltoluene	11.06	105	417221	41.31	ppb	95
88) 2-Chlorotoluene	11.01	91	340873	40.48	ppb	88
89) 1,3,5-Trimethylbenzene	11.12	105	382964	41.40	ppb	97
90) 4-Chlorotoluene	11.13	91	343947	40.60	ppb	99
91) Tert-Butylbenzene	11.44	119	234880	44.83	ppb	98
92) 1,2,4-Trimethylbenzene	11.49	105	396710	42.65	ppb	99
93) Sec-Butylbenzene	11.66	105	437165	44.90	ppb	99
94) p-Isopropyltoluene	11.81	119	441578	43.11	ppb	98
95) Benzyl Chloride	11.99	91	88019	35.87	ppb	99
96) 1,3-DCB	11.75	146	262502	43.48	ppb	98
97) 1,4-DCB	11.84	146	255429	43.91	ppb	96
98) n-Butylbenzene	12.22	91	282853	41.90	ppb	98
99) 1,2-DCB	12.21	146	253718	42.63	ppb	99
100) Hexachloroethane	12.46	117	65707	41.10	ppb	99
101) 1,2-Dibromo-3-chloropropan	12.99	75	22876	44.84	ppb	91
102) 1,2,4-Trichlorobenzene	13.81	180	113144	43.34	ppb	94
103) Hexachlorobutadiene	13.99	225	114209	42.64	ppb	98
104) Naphthalene	14.05	128	238304	52.27	ppb	99
105) 1,2,3-Trichlorobenzene	14.30	180	146469	44.67	ppb	90

Quantitation Report


Data File : M:\MAX\DATA\211015\1015M19.D
Acq On : 15 Oct 21 18:31
Sample : 40ug/L VOC STD 10/15/21
Misc : IS&S 8/4/21

Vial: 9
Operator: LP,DG,CH
Inst : Max
Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
Title : METHOD 8260B
Last Update : Sat Oct 16 14:01:48 2021
Response via : Initial Calibration

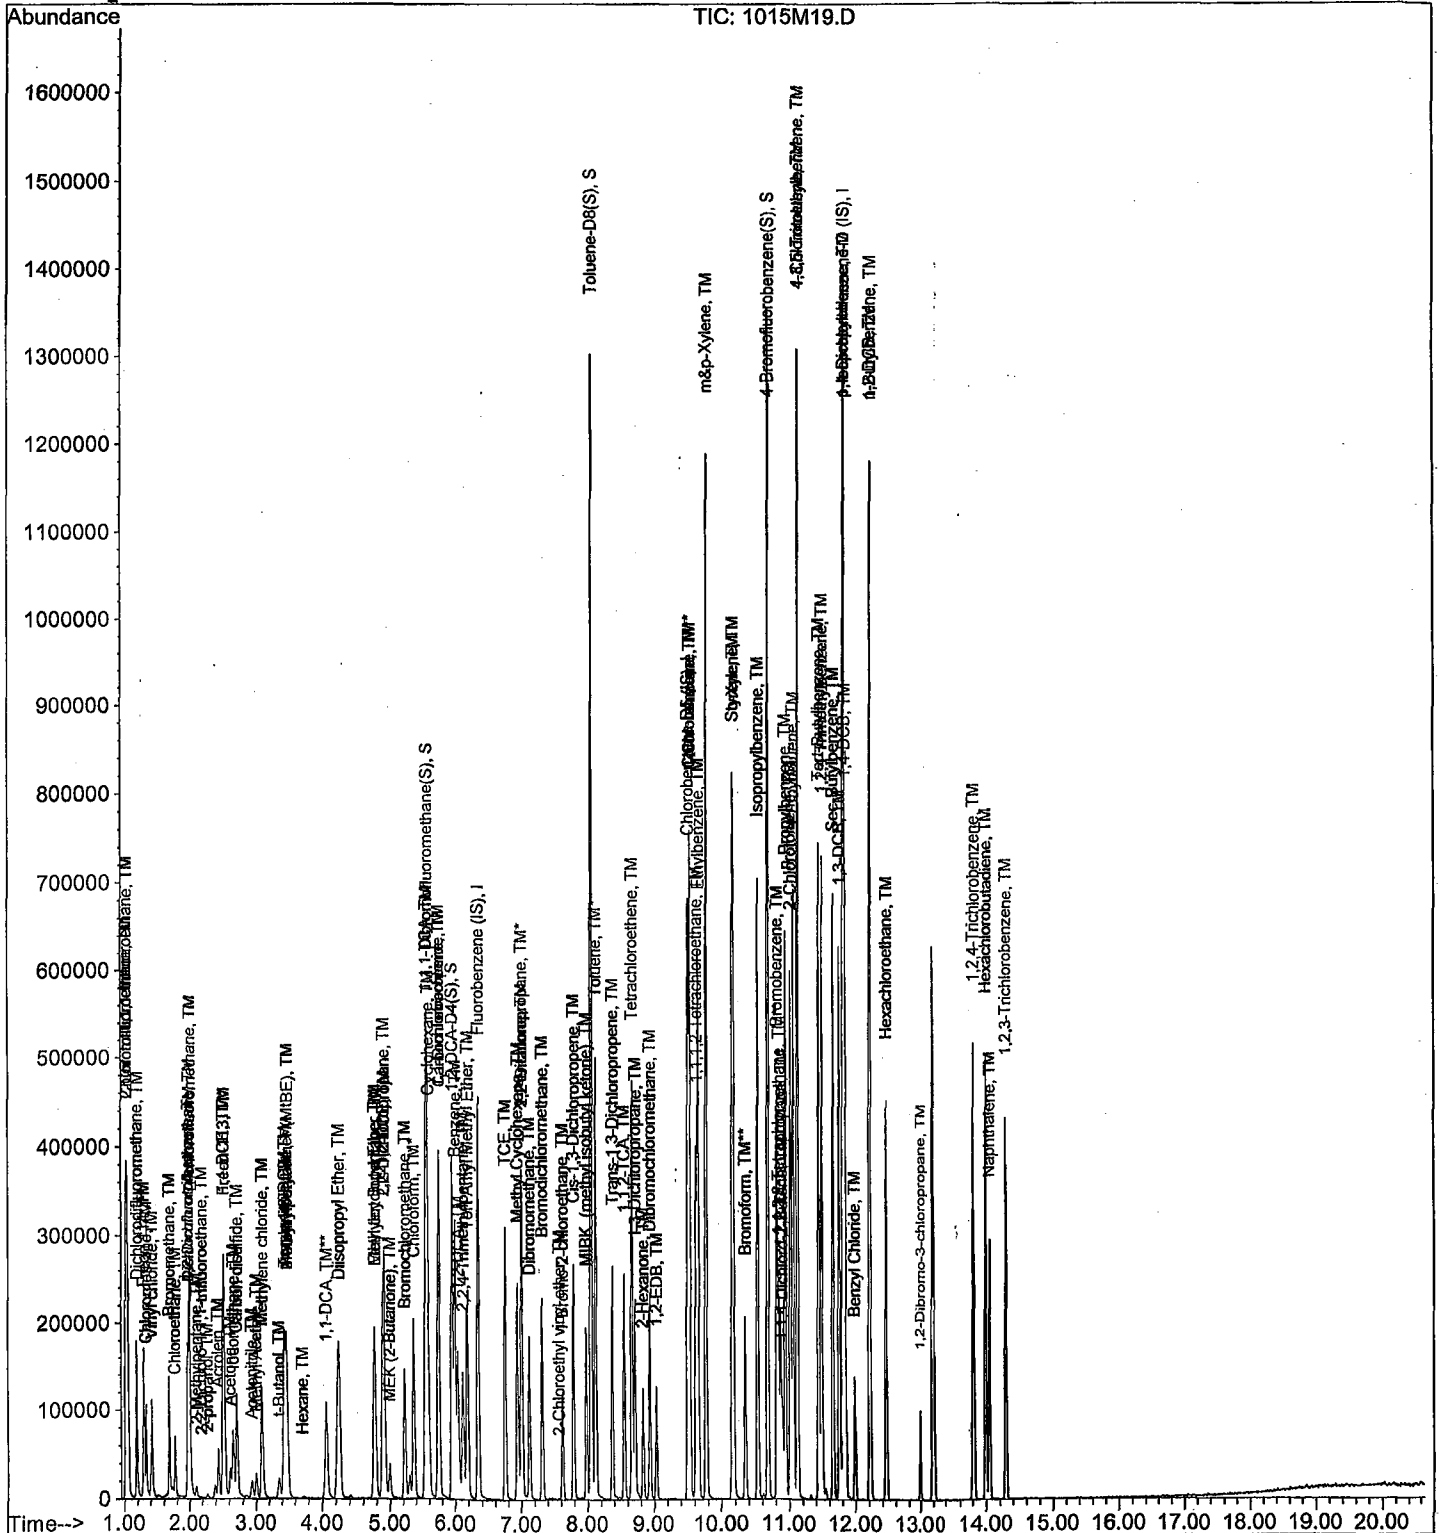

Data File : M:\MAX\DATA\211015\1015M20.D
 Acq On : 15 Oct 21 19:00
 Sample : 100ug/L VOC STD 10/15/21
 Misc : IS&S 8/4/21

Vial: 10
 Operator: LP, DG, CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 13:28:38 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.34	96	386789	25.00	ppb	0.00
65) Chlorobenzene-D5 (IS)	9.50	117	357810	25.00	ppb	0.00
80) 1,4-Dichlorobenzene-D (IS)	11.82	152	248989	25.00	ppb	0.00
System Monitoring Compounds						
41) Dibromofluoromethane(S)	5.56	111	442755	94.72	ppb	0.00
Spiked Amount	25.000		Recovery	=	378.876%	
46) 1,2-DCA-D4 (S)	5.95	65	315456	99.33	ppb	0.00
Spiked Amount	25.000		Recovery	=	397.320%	
66) Toluene-D8 (S)	8.05	98	1486255	91.76	ppb	0.00
Spiked Amount	25.000		Recovery	=	367.048%	
74) 4-Bromofluorobenzene(S)	10.68	95	657746	94.36	ppb	0.00
Spiked Amount	25.000		Recovery	=	377.452%	
Target Compounds						
2) Chlorotrifluoroethene	1.02	116	1201	7.92	ppb	# 45
3) Dichlorodifluoromethane	1.18	85	234560	119.53	ppb	99
4) Freon 114	1.29	85	146791	88.87	ppb	80
5) Chloromethane	1.33	50	143008	120.04	ppb	97
6) Vinyl chloride	1.42	62	168822	117.43	ppb	98
7) 2-Chloro-1,1,1-trifluoroet	1.00	118	1493	35.42	ppb	# 37
8) Bromomethane	1.68	94	135974	143.32	ppb	93
9) Chloroethane	1.76	64	126156	129.66	ppb	97
10) Dichlorofluoromethane	1.96	67	347423	106.00	ppb	100
11) Trichlorofluoromethane	1.99	101	454942	123.28	ppb	94
12) 2,2-Dichloro-1,1,1-trifluo	2.39	85	85	72.11	ppb	# 100
13) Acrolein	2.44	56	44550	122.70	ppb	88
14) Acetone	2.62	43	47910	108.58	ppb	94
15) Freon-113	2.52	151	175591	102.62	ppb	89
16) Acetonitrile	2.94	41	23864	193.35	ppb	91
17) 2-propanol	2.30	45	8518	465.81	ppb	92
18) 1,2-Dichlorotrifluoroethan	1.96	67	347584	106.03	ppb	# 100
19) 1,1-DCE	2.50	61	262927	116.95	ppb	95
20) t-Butanol	3.37	59	50833	214.24	ppb	99
21) Methyl Acetate	3.00	43	84654	106.53	ppb	85
22) Iodomethane	2.65	142	214716	120.36	ppb	98
23) Acrylonitrile	3.44	53	47089	105.86	ppb	93
24) 2-Methylpentane	2.09	71	220	93.32	ppb	# 100
25) Methylene chloride	3.08	84	160180	98.28	ppb	95
26) Carbon disulfide	2.71	76	194560	89.38	ppb	97
27) Methyl t-butyl ether (MtBE	3.47	73	555224	106.05	ppb	93
28) Trans-1,2-DCE	3.42	96	182546	121.83	ppb	100

(#) = qualifier out of range (m) = manual integration
 1015M20.D M1015W.M Wed Oct 20 12:06:45 2021

Data File : M:\MAX\DATA\211015\1015M20.D
 Acq On : 15 Oct 21 19:00
 Sample : 100ug/L VOC STD 10/15/21
 Misc : IS&S 8/4/21

Vial: 10
 Operator: LP, DG, CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 13:28:38 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
29) 3-Methylpentane	3.47	57	93951	112.00	ppb	89
30) Hexane	3.71	56	1846	87.00	ppb	# 100
31) Diisopropyl Ether	4.24	45	370710	102.14	ppb	97
32) 1,1-DCA	4.06	63	285289	106.17	ppb	# 93
34) Ethyl tert Butyl Ether	4.77	59	459729	96.83	ppb	97
35) Methylcyclopentane	4.77	56	17519	87.74	ppb	# 100
36) MEK (2-Butanone)	4.99	43	53511	103.84	ppb	90
37) Cis-1,2-DCE	4.91	96	197796	105.64	ppb	94
38) 2,2-Dichloropropane	4.89	77	346511	99.56	ppb	100
39) Chloroform	5.36	83	390282	106.18	ppb	94
40) Bromochloromethane	5.22	130	156085	115.65	ppb	# 88
42) 1,1,1-TCA	5.54	97	433213	112.79	ppb	97
43) Cyclohexane	5.58	41	121867	105.66	ppb	90
44) 1,1-Dichloropropene	5.75	75	231228	106.87	ppb	95
45) 2,2,4-Trimethylpentane	6.12	57	302605	88.31	ppb	87
47) Carbon Tetrachloride	5.74	117	411487	118.31	ppb	95
48) Tert Amyl Methyl Ether	6.18	73	450960	96.03	ppb	97
49) 1,2-DCA	6.04	62	367370	110.12	ppb	98
50) Benzene	5.99	78	649591	106.45	ppb	98
51) TCE	6.75	95	206061	115.34	ppb	84
52) 2-Pentanone	7.01	43	179595	209.77	ppb	99
53) 1,2-Dichloropropane	7.00	63	72296	113.59	ppb	96
54) Bromodichloromethane	7.31	83	317248	111.38	ppb	100
55) Methyl Cyclohexane	6.94	83	236830	106.31	ppb	93
56) Dibromomethane	7.12	93	119549	109.56	ppb	95
57) MIBK (methyl isobutyl ket	7.98	43	114125	97.99	ppb	98
58) 1-Bromo-2-chloroethane	7.62	144	42608	105.40	ppb	91
59) 2-Chloroethyl vinyl ether	7.69	43	19	15.45	ppb	# 100
60) Cis-1,3-Dichloropropene	7.79	75	293076	109.74	ppb	94
61) Toluene	8.12	91	786013	104.86	ppb	96
62) Trans-1,3-Dichloropropene	8.37	75	301333	109.95	ppb	100
63) 1,1,2-TCA	8.55	83	116902	99.29	ppb	93
64) 2-Hexanone	8.83	43	83212	100.16	ppb	# 92
67) 1,2-EDB	9.03	107	187298	116.98	ppb	98
68) Tetrachloroethene	8.66	164	163584	104.28	ppb	86
69) 1-Chlorohexane	9.53	91	140232	99.08	ppb	96
70) 1,1,1,2-Tetrachloroethane	9.62	131	281249	106.91	ppb	97
71) m&p-Xylene	9.77	106	823233	209.61	ppb	98
72) o-Xylene	10.16	106	418928	105.33	ppb	98
73) Styrene	10.18	104	692047	106.57	ppb	98
75) 1,3-Dichloropropane	8.71	76	259322	105.38	ppb	91
76) Dibromochloromethane	8.93	129	278663	112.70	ppb	98

(#) = qualifier out of range (m) = manual integration

Data File : M:\MAX\DATA\211015\1015M20.D
 Acq On : 15 Oct 21 19:00
 Sample : 100ug/L VOC STD 10/15/21
 Misc : IS&S 8/4/21

Vial: 10
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 13:28:38 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
77) Chlorobenzene	9.53	112	618681	102.72	ppb	96
78) Ethylbenzene	9.65	91	972119	107.04	ppb	100
79) Bromoform	10.35	173	247112	120.13	ppb	95
81) Isopropylbenzene	10.54	105	1132302	104.03	ppb	98
82) 1,1,2,2-Tetrachloroethane	10.85	83	183360	100.48	ppb	93
83) 1,2,3-Trichloropropane	10.88	110	96387	113.47	ppb	94
84) t-1,4-Dichloro-2-Butene	10.90	53	52050	92.63	ppb	80
85) Bromobenzene	10.81	156	374456	100.76	ppb	91
86) n-Propylbenzene	10.94	91	1150904	105.49	ppb	100
87) 4-Ethyltoluene	11.06	105	1068018	104.87	ppb	94
88) 2-Chlorotoluene	11.02	91	751088	88.44	ppb	92
89) 1,3,5-Trimethylbenzene	11.12	105	1000113	107.22	ppb	99
90) 4-Chlorotoluene	11.13	91	881242	103.15	ppb	99
91) Tert-Butylbenzene	11.44	119	615168	116.44	ppb	97
92) 1,2,4-Trimethylbenzene	11.49	105	1027302	109.19	ppb	98
93) Sec-Butylbenzene	11.66	105	1145861	116.71	ppb	100
94) p-Isopropyltoluene	11.81	119	1156691	111.42	ppb	99
95) Benzyl Chloride	11.99	91	250447	101.21	ppb	97
96) 1,3-DCB	11.75	146	675841	111.01	ppb	99
97) 1,4-DCB	11.85	146	672085	115.40	ppb	98
98) n-Butylbenzene	12.22	91	786990	114.02	ppb	97
99) 1,2-DCB	12.21	146	677640	112.91	ppb	98
100) Hexachloroethane	12.46	117	181188	112.65	ppb	98
101) 1,2-Dibromo-3-chloropropan	12.99	75	63114	121.24	ppb	93
102) 1,2,4-Trichlorobenzene	13.81	180	337280	123.99	ppb	90
103) Hexachlorobutadiene	13.99	225	307962	112.70	ppb	97
104) Naphthalene	14.06	128	746536	118.59	ppb	97
105) 1,2,3-Trichlorobenzene	14.30	180	462536	133.70	ppb	90

Quantitation Report


Data File : M:\MAX\DATA\211015\1015M20.D
Acq On : 15 Oct 21 19:00
Sample : 100ug/L VOC STD 10/15/21
Misc : IS&S 8/4/21

Vial: 10
Operator: LP,DG,CH
Inst : Max
Multiplr: 1.00

Quant Time: Oct 16 13:29 2021

Quant Results File: M1015W.RES

Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
Title : METHOD 8260B
Last Update : Sat Oct 16 14:01:48 2021
Response via : Initial Calibration

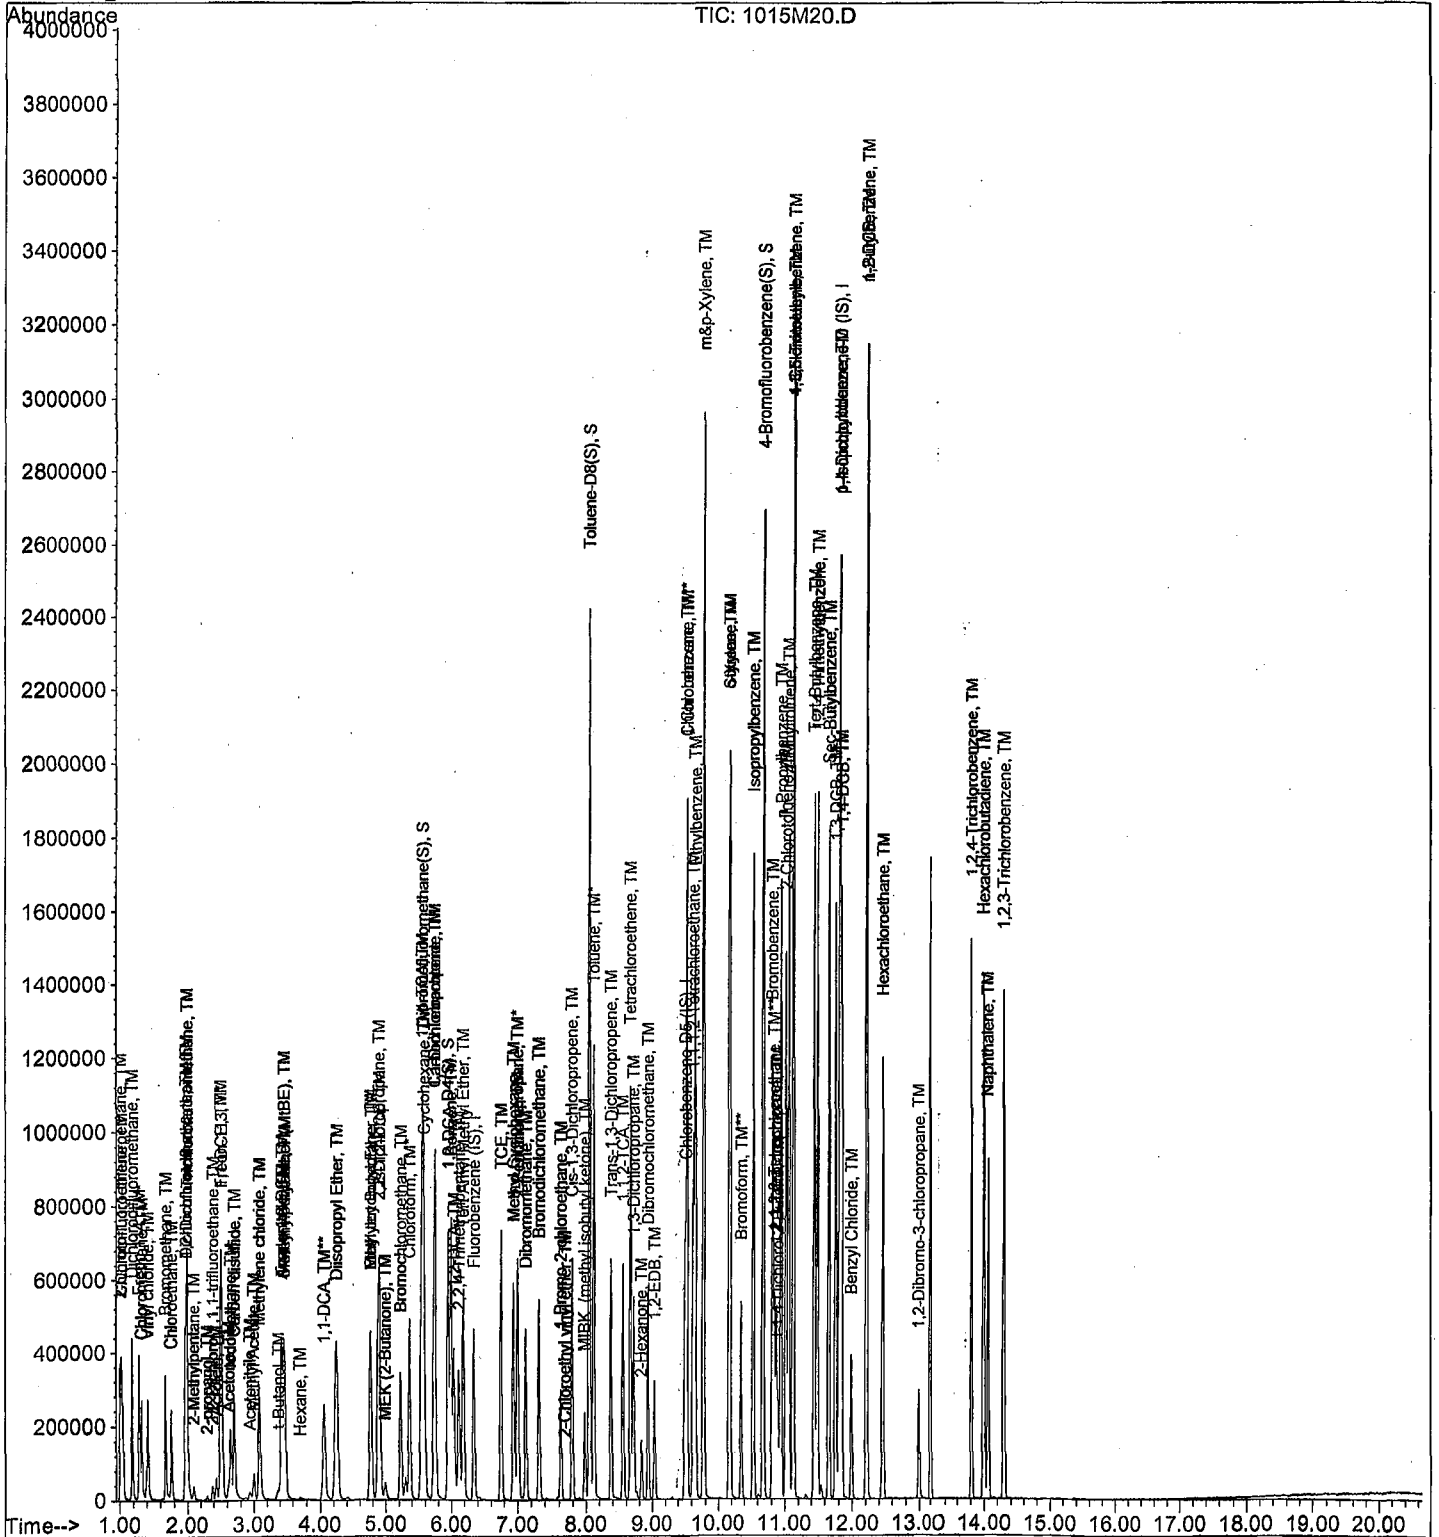

VOLATILE ORGANIC ANALYSIS BY
EPA METHOD 8260B

Form 7

Second Source Calibration

Lab Name: APPL, Inc.
Case No: _____
Matrix: Water

SDG No: _____
Date Analyzed: 10/15/2021
Instrument: Max
Initial Cal. Date: 10/15/2021
Data File: 1015M22.D

		Compound	MEAN	CCRF	%D	%Drift
1	TM	Chlorotrifluoroethene	0.0000	0.0122	0.00	TM
2	TM	Dichlorodifluoromethane	0.1497	0.1425	4.8	TM
3	TM	Freon 114	0.0839	0.0990	18	TM
4	TM**	Chloromethane	0.0893	0.0842	5.7	TM**
5	TM*	Vinyl chloride	0.1101	0.1001	9.1	TM*
6	TM	2-Chloro-1,1,1-trifluoroethane	0.0000	0.0024	0.00	TM
7	TM	Bromomethane	0.0931	0.0814	13	TM
8	TML	Chloroethane	0.0844	0.0648	23	TML 8.2
9	TM	Dichlorofluoromethane	0.2416	0.1948	19	TM
10	TM	Trichlorofluoromethane	0.2889	0.2752	4.8	TM
11	TM	2,2-Dichloro-1,1,1-trifluoroethane	0.0000	0.0001	0.00	TM
12	TMQ	Acrolein	0.0145	0.0122	15	TMQ 12
13	TM	Acetone	0.0326	0.0319	2.1	TM
14	TM	Freon-113	0.1176	0.1116	5.1	TM
15	TM	Acetonitrile	0.0077	0.0083	7.5	TM
16	TML	2-propanol	0.0000	0.0009	0.00	TML
17	TM	1,2-Dichlorotrifluoroethane	0.2416	0.1948	19	TM
18	TM*	1,1-DCE	0.1751	0.1607	8.2	TM*
19	TMQ	t-Butanol	0.0101	0.0116	14	TMQ 16
20	TMQ	Methyl Acetate	0.0528	0.0415	21	TMQ 24 *NT
21	TML	Iodomethane	0.1096	0.0881	20	TML 24 *NT
22	TML	Acrylonitrile	0.0252	0.0300	19	TML 2.8
23	TM	Methylene chloride	0.1130	0.1086	3.9	TM
24	TM	Carbon disulfide	0.1424	0.1277	10	TM
25	TM	Methyl t-butyl ether (MtBE)	0.3769	0.3493	7.3	TM
26	TM	Trans-1,2-DCE	0.1221	0.1176	3.6	TM
27	TML	3-Methylpentane	0.0702	0.0590	16	TML 7.9
28	TM	Hexane	0.0000	0.0008	0.00	TM
29	TM	Diisopropyl Ether	0.2351	0.2190	6.9	TM
30	TM**	1,1-DCA	0.1831	0.1889	3.2	TM**
31	TM	Ethyl tert Butyl Ether	0.3021	0.2803	7.2	TM
32	TML	Methylcyclopentane	0.0160	0.0145	9.4	TML 13
33	TM	MEK (2-Butanone)	0.0341	0.0344	1.0	TM
34	TM	Cis-1,2-DCE	0.1352	0.1221	9.7	TM
35	TM	2,2-Dichloropropane	0.2349	0.2108	10	TM
36	TM*	Chloroform	0.2377	0.2410	1.4	TM*
37	TML	Bromochloromethane	0.1040	0.0967	7.0	TML 9.0
38	TM	1,1,1-TCA	0.2791	0.2799	0.27	TM
39	TM	Cyclohexane	0.0798	0.0682	15	TM
40	TM	1,1-Dichloropropene	0.1514	0.1477	2.5	TM

Average

8.6

VOLATILE ORGANIC ANALYSIS BY
EPA METHOD 8260B

Form 7

Second Source Calibration

Lab Name: APPL, Inc.
Case No: _____
Matrix: Water

SDG No: _____
Date Analyzed: 10/15/2021
Instrument: Max
Cal. Date: 10/15/2021
Data File: 1015M22.D

		Compound	MEAN	CCRF	%D	%Drift	
41	TM	2,2,4-Trimethylpentane	0.1964	0.1702	13	TM	
42	TM	Carbon Tetrachloride	0.2625	0.2517	4.1	TM	
43	TM	Tert Amyl Methyl Ether	0.2978	0.2793	6.2	TM	
44	TM	1,2-DCA	0.2350	0.2325	1.1	TM	
45	TM	Benzene	0.4384	0.4137	5.6	TM	
46	TM	TCE	0.1404	0.1388	1.1	TM	
47	TM	2-Pentanone	0.0570	0.0572	0.40	TM	
48	TM*L	1,2-Dichloropropane	0.0476	0.0463	2.9	TM*L	5.1
49	TM	Bromodichloromethane	0.1968	0.1954	0.72	TM	
50	TML	Methyl Cyclohexane	0.1542	0.1469	4.7	TML	2.6
51	TM	Dibromomethane	0.0856	0.0761	11	TM	
52	TM	MIBK (methyl isobutyl ketone)	0.0729	0.0782	7.3	TM	
53	TML	1-Bromo-2-chloroethane	0.0245	0.0257	4.8	TML	6.7
54	TM	2-Chloroethyl vinyl ether	0.0000	0.0001	0.00	TM	
55	TM	Cis-1,3-Dichloropropene	0.1763	0.1779	0.88	TM	
56	TM*	Toluene	0.5070	0.4972	1.9	TM*	
57	TM	Trans-1,3-Dichloropropene	0.1749	0.1751	0.15	TM	
58	TM	1,1,2-TCA	0.0786	0.0760	3.3	TM	
59	TM	2-Hexanone	0.0493	0.0526	6.7	TM	
60	TM	1,2-EDB	0.1319	0.1272	3.6	TM	
61	TML	Tetrachloroethene	0.2207	0.1356	39	TML	4.5
62	TM	1-Chlorohexane	0.0992	0.0866	13	TM	
63	TM	1,1,1,2-Tetrachloroethane	0.1860	0.1885	1.4	TM	
64	TM	m&p-Xylene	0.2826	0.2811	0.55	TM	
65	TM	o-Xylene	0.2964	0.2821	4.8	TM	
66	TM	Styrene	0.4463	0.4632	3.8	TM	
67	TM	1,3-Dichloropropane	0.1940	0.1840	5.1	TM	
68	TM	Dibromochloromethane	0.1941	0.1947	0.35	TM	
69	TM**	Chlorobenzene	0.4334	0.4155	4.1	TM**	
70	TM*	Ethylbenzene	0.6860	0.6607	3.7	TM*	
71	TM**	Bromoform	0.1611	0.1543	4.2	TM**	
72	TM	Isopropylbenzene	1.166	1.132	2.9	TM	
73	TM**	1,1,2,2-Tetrachloroethane	0.2001	0.1827	8.7	TM**	
74	TM	1,2,3-Trichloropropane	0.1000	0.1008	0.81	TM	
75	TML	t-1,4-Dichloro-2-Butene	0.0601	0.0488	19	TML	4.0
76	TM	Bromobenzene	0.3816	0.3657	4.2	TM	
77	TM	n-Propylbenzene	1.151	1.138	1.2	TM	
78	TM	4-Ethyltoluene	1.063	0.9969	6.2	TM	
79	TM	2-Chlorotoluene	0.9129	0.8702	4.7	TM	
80	TM	1,3,5-Trimethylbenzene	0.9948	1.004	0.90	TM	

Average

5.2

VOLATILE ORGANIC ANALYSIS BY
EPA METHOD 8260B

Form 7

Second Source Calibration

Lab Name: APPL, Inc.

SDG No: _____

Case No: _____

Date Analyzed: 10/15/2021

Matrix: Water

Instrument: Max

Cal. Date: 10/15/2021

Data File: 1015M22.D

		Compound	MEAN	CCRF	%D	%Drift
81	TM	4-Chlorotoluene	0.9068	0.8859	2.3	TM
82	TM	Tert-Butylbenzene	0.5492	0.5705	3.9	TM
83	TM	1,2,4-Trimethylbenzene	0.9425	0.9915	5.2	TM
84	TM	Sec-Butylbenzene	1.051	1.108	5.5	TM
85	TM	p-Isopropyltoluene	1.016	1.070	5.3	TM
86	TM	Benzyl Chloride	0.2406	0.2024	16	TM
87	TM	1,3-DCB	0.6644	0.6756	1.7	TM
88	TM	1,4-DCB	0.6767	0.6541	3.3	TM
89	TML	n-Butylbenzene	0.5721	0.6278	9.7	TML 7.4
90	TM	1,2-DCB	0.6504	0.6356	2.3	TM
91	TM	Hexachloroethane	0.1703	0.1719	0.98	TM
92	TML	1,2-Dibromo-3-chloropropane	0.0437	0.0485	11	TML 13
93	TML	1,2,4-Trichlorobenzene	0.1936	0.2049	5.8	TML 17
94	TML	Hexachlorobutadiene	0.2401	0.2482	3.4	TML 9.7
95	TMQ	Naphthalene	0.4088	0.4281	4.7	TMQ 8.9
96	TML	1,2,3-Trichlorobenzene	0.2371	0.2821	19	TML 13
97						
98						
99						
100						
101						
102						
103						
104						
105						
106						
107						
108						
109						
110						
111						
112						
113						
114						
115						
116						
117						
118						
119						
120						

Average

6.3

Data File : M:\MAX\DATA\211015\1015M22.D
 Acq On : 15 Oct 21 19:57
 Sample : (SS) 10ug/L VOC STD 10/15/21
 Misc : IS&S 8/4/21

Vial: 12
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 16 14:01 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 14:01:48 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.34	96	407759	25.00	ppb	0.00
65) Chlorobenzene-D5 (IS)	9.50	117	364241	25.00	ppb	0.00
80) 1,4-Dichlorobenzene-D (IS)	11.82	152	235667	25.00	ppb	0.00

System Monitoring Compounds

41) Dibromofluoromethane(S)	5.56	111	123620	24.41	ppb	0.00
Spiked Amount	25.000		Recovery	=	97.644%	
46) 1,2-DCA-D4(S)	5.95	65	86328	24.44	ppb	0.00
Spiked Amount	25.000		Recovery	=	97.764%	
66) Toluene-D8(S)	8.05	98	412111	24.62	ppb	0.00
Spiked Amount	25.000		Recovery	=	98.464%	
74) 4-Bromofluorobenzene(S)	10.68	95	166312	24.60	ppb	0.00
Spiked Amount	25.000		Recovery	=	98.388%	

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Dichlorodifluoromethane	1.18	85	23248	9.52	ppb	98
4) Freon 114	1.29	85	16154	11.81	ppb	81
5) Chloromethane	1.33	50	13730	9.43	ppb	91
6) Vinyl chloride	1.42	62	16330	9.09	ppb	99
8) Bromomethane	1.68	94	13271	8.74	ppb	98
9) Chloroethane	1.77	64	10562	9.18	ppb	92
10) Dichlorofluoromethane	1.97	67	31774	8.06	ppb	97
11) Trichlorofluoromethane	2.00	101	44881	9.52	ppb	96
13) Acrolein	2.44	56	24941	109.40	ppb	90
14) Acetone	2.61	43	26025	48.95	ppb	99
15) Freon-113	2.52	151	18195	9.49	ppb	94
16) Acetonitrile	2.93	41	16970	134.32	ppb	90
18) 1,2-Dichlorotrifluoroethan	1.97	67	31774	8.06	ppb	100
19) 1,1-DCE	2.51	61	26210	9.18	ppb	99
20) t-Butanol	3.34	59	23571	144.72	ppb	93
21) Methyl Acetate	2.99	43	6766	7.57	ppb	95
22) Iodomethane	2.66	142	14370	7.58	ppb	95
23) Acrylonitrile	3.43	53	4893	9.72	ppb	91
25) Methylene chloride	3.08	84	17714	9.61	ppb	94
26) Carbon disulfide	2.71	76	20832	8.97	ppb	# 92
27) Methyl t-butyl ether (MtBE)	3.47	73	56980	9.27	ppb	92
28) Trans-1,2-DCE	3.43	96	19186	9.64	ppb	92
29) 3-Methylpentane	3.46	57	9624	9.21	ppb	# 87
31) Diisopropyl Ether	4.24	45	35716	9.31	ppb	90
32) 1,1-DCA	4.06	63	30810	10.32	ppb	95
34) Ethyl tert Butyl Ether	4.77	59	45712	9.28	ppb	96
35) Methylcyclopentane	4.78	56	2359	11.28	ppb	100

(#) = qualifier out of range (m) = manual integration

Data File : M:\MAX\DATA\211015\1015M22.D
 Acq On : 15 Oct 21 19:57
 Sample : (SS) 10ug/L VOC STD 10/15/21
 Misc : IS&S 8/4/21

Vial: 12
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 16 14:01 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 14:01:48 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
36) MEK (2-Butanone)	4.99	43	28077	50.51	ppb	# 93
37) Cis-1,2-DCE	4.91	96	19914	9.03	ppb	92
38) 2,2-Dichloropropane	4.89	77	34376	8.97	ppb	97
39) Chloroform	5.36	83	39302	10.14	ppb	97
40) Bromochloromethane	5.22	130	15775	9.10	ppb	95
42) 1,1,1-TCA	5.54	97	45646	10.03	ppb	94
43) Cyclohexane	5.59	41	11131	8.55	ppb	86
44) 1,1-Dichloropropene	5.75	75	24083	9.75	ppb	95
45) 2,2,4-Trimethylpentane	6.12	57	27765	8.67	ppb	86
47) Carbon Tetrachloride	5.74	117	41049	9.59	ppb	95
48) Tert Amyl Methyl Ether	6.18	73	45547	9.38	ppb	96
49) 1,2-DCA	6.04	62	37921	9.89	ppb	97
50) Benzene	5.99	78	67483	9.44	ppb	96
51) TCE	6.75	95	22638	9.89	ppb	91
52) 2-Pentanone	7.01	43	116600	125.50	ppb	100
53) 1,2-Dichloropropane	7.00	63	7545	9.49	ppb	# 91
54) Bromodichloromethane	7.31	83	31868	9.93	ppb	97
55) Methyl Cyclohexane	6.94	83	23967	9.74	ppb	90
56) Dibromomethane	7.12	93	12407	8.88	ppb	93
57) MIBK (methyl isobutyl ket	7.98	43	63733	53.64	ppb	95
58) 1-Bromo-2-chloroethane	7.62	144	4192	9.33	ppb	75
60) Cis-1,3-Dichloropropene	7.79	75	29014	10.09	ppb	96
61) Toluene	8.12	91	81096	9.81	ppb	99
62) Trans-1,3-Dichloropropene	8.37	75	28562	10.02	ppb	97
63) 1,1,2-TCA	8.55	83	12396	9.67	ppb	88
64) 2-Hexanone	8.83	43	42858	53.33	ppb	97
67) 1,2-EDB	9.03	107	18534	9.64	ppb	93
68) Tetrachloroethene	8.66	164	19760	10.45	ppb	# 76
69) 1-Chlorohexane	9.53	91	12619	8.73	ppb	96
70) 1,1,1,2-Tetrachloroethane	9.62	131	27467	10.14	ppb	93
71) m&p-Xylene	9.77	106	81898	19.89	ppb	97
72) o-Xylene	10.16	106	41097	9.52	ppb	90
73) Styrene	10.18	104	67486	10.38	ppb	# 95
75) 1,3-Dichloropropane	8.71	76	26810	9.49	ppb	92
76) Dibromochloromethane	8.93	129	28373	10.03	ppb	98
77) Chlorobenzene	9.53	112	60543	9.59	ppb	98
78) Ethylbenzene	9.65	91	96264	9.63	ppb	99
79) Bromoform	10.35	173	22475	9.58	ppb	89
81) Isopropylbenzene	10.53	105	106724	9.71	ppb	99
82) 1,1,2,2-Tetrachloroethane	10.84	83	17225	9.13	ppb	# 88
83) 1,2,3-Trichloropropane	10.87	110	9505	10.08	ppb	85
84) t-1,4-Dichloro-2-Butene	10.90	53	4599	9.60	ppb	75

(#) = qualifier out of range (m) = manual integration

Data File : M:\MAX\DATA\211015\1015M22.D
 Acq On : 15 Oct 21 19:57
 Sample : (SS) 10ug/L VOC STD 10/15/21
 Misc : IS&S 8/4/21

Vial: 12
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 16 14:01 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 14:01:48 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
85) Bromobenzene	10.81	156	34477	9.58	ppb	91
86) n-Propylbenzene	10.94	91	107263	9.88	ppb	94
87) 4-Ethyltoluene	11.06	105	93970	9.38	ppb	94
88) 2-Chlorotoluene	11.01	91	82030	9.53	ppb	94
89) 1,3,5-Trimethylbenzene	11.12	105	94620	10.09	ppb	96
90) 4-Chlorotoluene	11.13	91	83509	9.77	ppb	98
91) Tert-Butylbenzene	11.44	119	53776	10.39	ppb	96
92) 1,2,4-Trimethylbenzene	11.49	105	93466	10.52	ppb	98
93) Sec-Butylbenzene	11.66	105	104477	10.55	ppb	99
94) p-Isopropyltoluene	11.81	119	100883	10.53	ppb	97
95) Benzyl Chloride	11.99	91	19077	8.41	ppb	97
96) 1,3-DCB	11.75	146	63689	10.17	ppb	94
97) 1,4-DCB	11.84	146	61660	9.67	ppb	97
98) n-Butylbenzene	12.22	91	59181	9.26	ppb	96
99) 1,2-DCB	12.21	146	59914	9.77	ppb	96
100) Hexachloroethane	12.46	117	16207	10.10	ppb	91
101) 1,2-Dibromo-3-chloropropan	12.99	75	4572	8.68	ppb #	90
102) 1,2,4-Trichlorobenzene	13.81	180	19312	8.25	ppb	89
103) Hexachlorobutadiene	13.99	225	23401	9.03	ppb	92
104) Naphthalene	14.06	128	40355	9.11	ppb	99
105) 1,2,3-Trichlorobenzene	14.30	180	26595	8.69	ppb	90

Quantitation Report


Data File : M:\MAX\DATA\211015\1015M22.D
Acq On : 15 Oct 21 19:57
Sample : (SS) 10ug/L VOC STD 10/15/21
Misc : IS&S 8/4/21

Vial: 12
Operator: LP,DG,CH
Inst : Max
Multiplr: 1.00

Quant Time: Oct 16 14:01 2021

Quant Results File: M1015W.RES

Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
Title : METHOD 8260B
Last Update : Sat Oct 16 14:01:48 2021
Response via : Initial Calibration

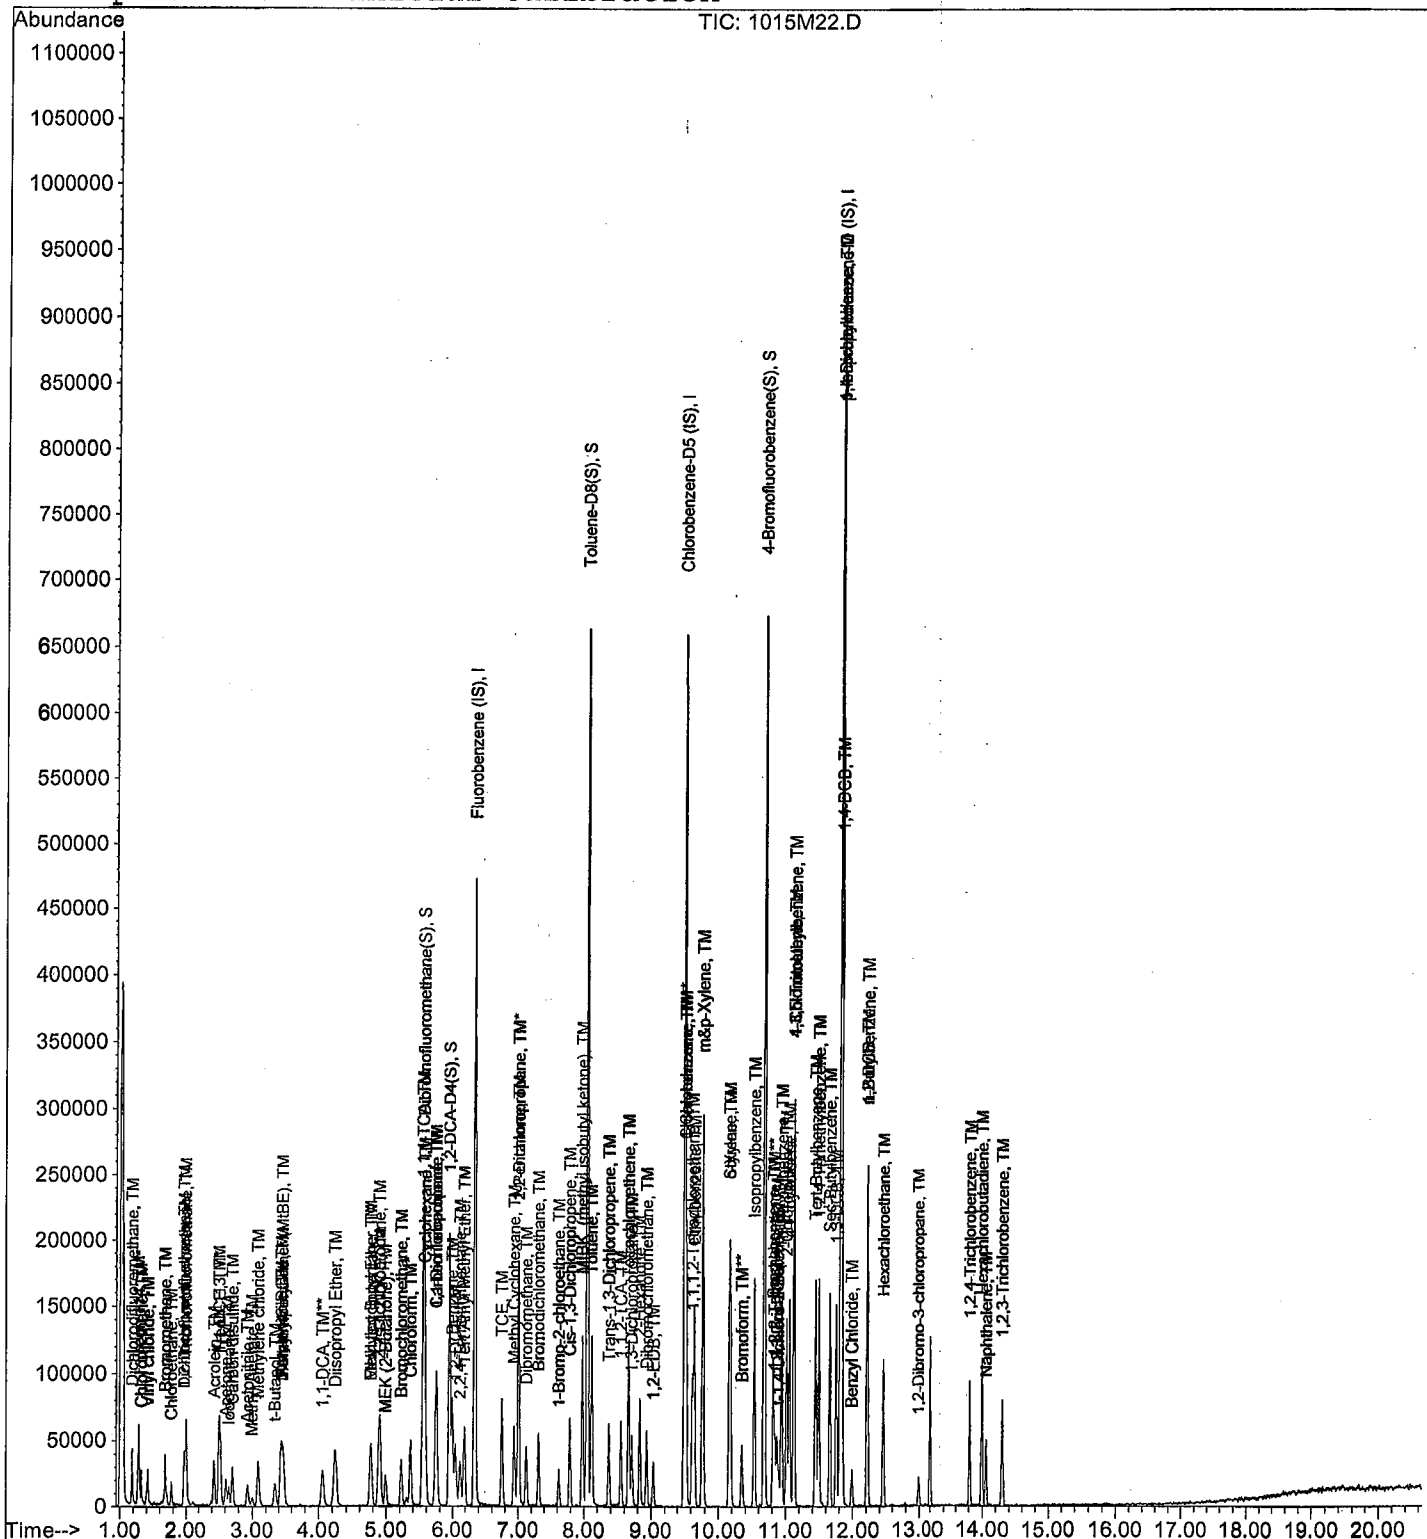

VOLATILE ORGANIC ANALYSIS BY
EPA METHOD 8260B

Form 7

Continuing Calibration

Lab Name: APPL, Inc.
Case No: _____
Matrix: Water

SDG No: _____
Date Analyzed: 10/26/2021
Instrument: Max
Initial Cal. Date: 10/15/2021
Data File: 1026M25.D

		Compound	MEAN	CCRF	%D	%Drift	
1	I	Fluorobenzene (IS)	ISTD				I
2	TM	Chlorotrifluoroethene	0.0000	0.0127	0.00		TM
3	TM	Dichlorodifluoromethane	0.1497	0.1261	16		TM
4	TM	Freon 114	0.0839	0.0932	11		TM
5	TM**	Chloromethane	0.0893	0.0752	16		TM**
6	TM*	Vinyl chloride	0.1101	0.0848	23		TM*
7	TM	2-Chloro-1,1,1-trifluoroethane	0.0000	0.0018	0.00		TM
8	TM	Bromomethane	0.0931	0.0885	4.9		TM
9	TML	Chloroethane	0.0844	0.0640	24	9.1	TML
10	TM	Dichlorofluoromethane	0.2416	0.2372	1.8		TM
11	TM	Trichlorofluoromethane	0.2889	0.2637	8.7		TM
12	TM	2,2-Dichloro-1,1,1-trifluoroethane	0.0000	0.0001	0.00		TM
13	TMQ	Acrolein	0.0145	0.0119	18		TMQ 15
14	TM	Acetone	0.0326	0.0302	7.2		TM
15	TM	Freon-113	0.1176	0.1173	0.22		TM
16	TM	Acetonitrile	0.0077	0.0077	0.41		TM
17	TML	2-propanol	0.0000	0.0010	0.00		TML
18	TM	1,2-Dichlorotrifluoroethane	0.2416	0.2372	1.8		TM
19	TM*	1,1-DCE	0.1751	0.1730	1.2		TM*
20	TMQ	t-Butanol	0.0101	0.0108	6.2		TMQ 6.7
21	TMQ	Methyl Acetate	0.0528	0.0488	7.6		TMQ 11
22	TML	Iodomethane	0.1096	0.0963	12		TML 18
23	TML	Acrylonitrile	0.0252	0.0308	22	0.02	TML
24	TM	2-Methylpentane	0.0000	0.0004	0.00		TM
25	TM	Methylene chloride	0.1130	0.1079	4.5		TM
26	TM	Carbon disulfide	0.1424	0.1362	4.3		TM
27	TM	Methyl t-butyl ether (MtBE)	0.3769	0.3602	4.4		TM
28	TM	Trans-1,2-DCE	0.1221	0.1160	5.0		TM
29	TML	3-Methylpentane	0.0702	0.0681	2.9	7.1	TML
30	TM	Hexane	0.0000	0.0001	0.00		TM
31	TM	Diisopropyl Ether	0.2351	0.2432	3.5		TM
32	TM**	1,1-DCA	0.1831	0.1855	1.3		TM**
33	TM	Ethyl tert Butyl Ether	0.3021	0.3001	0.65		TM
34	TML	Methylcyclopentane	0.0160	0.0010	94	105	TML
35	TM	MEK (2-Butanone)	0.0341	0.0349	2.4		TM
36	TM	Cis-1,2-DCE	0.1352	0.1276	5.6		TM
37	TM	2,2-Dichloropropane	0.2349	0.2137	9.0		TM
38	TM*	Chloroform	0.2377	0.2532	6.5		TM*
39	TML	Bromochloromethane	0.1040	0.0984	5.4	7.3	TML
40	S	Dibromofluoromethane(S)	0.3105	0.3246	4.6		S
Average					8.6		

VOLATILE ORGANIC ANALYSIS BY
EPA METHOD 8260B

Form 7

Continuing Calibration

Lab Name: APPL, Inc.
Case No: _____
Matrix: Water

SDG No: _____
Date Analyzed: 10/26/2021
Instrument: Max
Cal. Date: 10/15/2021
Data File: 1026M25.D

		Compound	MEAN	CCRF	%D	%Drift
41	TM	1,1,1-TCA	0.2791	0.2873	2.9	TM
42	TM	Cyclohexane	0.0798	0.0831	4.1	TM
43	TM	1,1-Dichloropropene	0.1514	0.1489	1.7	TM
44	TM	2,2,4-Trimethylpentane	0.1964	0.1880	4.3	TM
45	S	1,2-DCA-D4(S)	0.2166	0.2158	0.33	S
46	TM	Carbon Tetrachloride	0.2625	0.2628	0.10	TM
47	TM	Tert Amyl Methyl Ether	0.2978	0.2847	4.4	TM
48	TM	1,2-DCA	0.2350	0.2284	2.8	TM
49	TM	Benzene	0.4384	0.4119	6.0	TM
50	TM	TCE	0.1404	0.1294	7.8	TM
51	TM	2-Pentanone	0.0570	0.0572	0.49	TM
52	TM*L	1,2-Dichloropropane	0.0476	0.0471	1.1	TM*L 3.4
53	TM	Bromodichloromethane	0.1968	0.1951	0.88	TM
54	TML	Methyl Cyclohexane	0.1542	0.1417	8.1	TML 6.0
55	TM	Dibromomethane	0.0856	0.0768	10	TM
56	TM	MIBK (methyl isobutyl ketone)	0.0729	0.0750	2.9	TM
57	TML	1-Bromo-2-chloroethane	0.0245	0.0258	5.4	TML 6.1
58	TM	2-Chloroethyl vinyl ether	0.0000	0.0000	0.00	TM
59	TM	Cis-1,3-Dichloropropene	0.1763	0.1753	0.61	TM
60	TM*	Toluene	0.5070	0.4841	4.5	TM*
61	TM	Trans-1,3-Dichloropropene	0.1749	0.1676	4.2	TM
62	TM	1,1,2-TCA	0.0786	0.0723	8.0	TM
63	TM	2-Hexanone	0.0493	0.0505	2.4	TM
64	I	Chlorobenzene-D5 (IS)	ISTD			I
65	S	Toluene-D8(S)	1.149	1.171	1.9	S
66	TM	1,2-EDB	0.1319	0.1206	8.6	TM
67	TML	Tetrachloroethene	0.2207	0.1086	51	TML 19
68	TM	1-Chlorohexane	0.0992	0.0829	16	TM
69	TM	1,1,1,2-Tetrachloroethane	0.1860	0.2021	8.7	TM
70	TM	m&p-Xylene	0.2826	0.2891	2.3	TM
71	TM	o-Xylene	0.2964	0.2808	5.3	TM
72	TM	Styrene	0.4463	0.4507	0.99	TM
73	S	4-Bromofluorobenzene(S)	0.4641	0.4762	2.6	S
74	TM	1,3-Dichloropropane	0.1940	0.1851	4.6	TM
75	TM	Dibromochloromethane	0.1941	0.1905	1.8	TM
76	TM**	Chlorobenzene	0.4334	0.4342	0.18	TM**
77	TM*	Ethylbenzene	0.6860	0.6876	0.24	TM*
78	TM**	Bromoform	0.1611	0.1553	3.6	TM**
79	I	1,4-Dichlorobenzene-D (IS)	ISTD			I
80	TM	Isopropylbenzene	1.166	1.143	2.0	TM

Average

5.1

VOLATILE ORGANIC ANALYSIS BY
EPA METHOD 8260B

Form 7

Continuing Calibration

Lab Name: APPL, Inc.
Case No: _____
Matrix: Water

SDG No: _____
Date Analyzed: 10/26/2021
Instrument: Max
Cal. Date: 10/15/2021
Data File: 1026M25.D

		Compound	MEAN	CCRF	%D	%Drift
81	TM**	1,1,2,2-Tetrachloroethane	0.2001	0.1881	7.0	TM**
82	TM	1,2,3-Trichloropropane	0.1000	0.0983	1.7	TM
83	TML	t-1,4-Dichloro-2-Butene	0.0601	0.0534	11	TML 4.8
84	TM	Bromobenzene	0.3816	0.3709	2.8	TM
85	TM	n-Propylbenzene	1.151	1.121	2.7	TM
86	TM	4-Ethyltoluene	1.063	1.067	0.35	TM
87	TM	2-Chlorotoluene	0.9129	0.8933	2.1	TM
88	TM	1,3,5-Trimethylbenzene	0.9948	1.008	1.3	TM
89	TM	4-Chlorotoluene	0.9068	0.8731	3.7	TM
90	TM	Tert-Butylbenzene	0.5492	0.5839	6.3	TM
91	TM	1,2,4-Trimethylbenzene	0.9425	0.9649	2.4	TM
92	TM	Sec-Butylbenzene	1.051	1.103	5.0	TM
93	TM	p-Isopropyltoluene	1.016	1.032	1.6	TM
94	TM	Benzyl Chloride	0.2406	0.1893	21	TM *NT
95	TM	1,3-DCB	0.6644	0.6525	1.8	TM
96	TM	1,4-DCB	0.6767	0.6619	2.2	TM
97	TML	n-Butylbenzene	0.5721	0.6095	6.5	TML 9.7
98	TM	1,2-DCB	0.6504	0.6278	3.5	TM
99	TM	Hexachloroethane	0.1703	0.1831	7.5	TM
100	TML	1,2-Dibromo-3-chloropropane	0.0437	0.0469	7.2	TML 16
101	TML	1,2,4-Trichlorobenzene	0.1936	0.2153	11	TML 14
102	TML	Hexachlorobutadiene	0.2401	0.2444	1.8	TML 11
103	TMQ	Naphthalene	0.4088	0.3833	6.2	TMQ 17
104	TML	1,2,3-Trichlorobenzene	0.2371	0.2671	13	TML 16
105						
106						
107						
108						
109						
110						
111						
112						
113						
114						
115						
116						
117						
118						
119						
120						

Average

5.4

Data File : M:\MAX\DATA\211015\1026M25.D
 Acq On : 26 Oct 21 20:30
 Sample : 211026B CCV 10ug/L
 Misc : IS&S 8/4/21

Vial: 25
 Operator: LP, DG, CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 27 7:38 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 14:01:48 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.37	96	386002	25.00	ppb	0.03
65) Chlorobenzene-D5 (IS)	9.53	117	343919	25.00	ppb	0.03
80) 1,4-Dichlorobenzene-D (IS)	11.85	152	227821	25.00	ppb	0.03

System Monitoring Compounds

41) Dibromofluoromethane (S)	5.59	111	125304	26.14	ppb	0.03
Spiked Amount	25.000		Recovery	= 104.552%		
46) 1,2-DCA-D4 (S)	5.98	65	83312	24.92	ppb	0.03
Spiked Amount	25.000		Recovery	= 99.664%		
66) Toluene-D8 (S)	8.08	98	402827	25.48	ppb	0.03
Spiked Amount	25.000		Recovery	= 101.936%		
74) 4-Bromofluorobenzene (S)	10.70	95	163778	25.65	ppb	0.03
Spiked Amount	25.000		Recovery	= 102.612%		

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Dichlorodifluoromethane	1.20	85	19464	8.42	ppb	98
4) Freon 114	1.30	85	14390	11.11	ppb	77
5) Chloromethane	1.34	50	11611	8.42	ppb	88
6) Vinyl chloride	1.43	62	13093	7.70	ppb	100
8) Bromomethane	1.69	94	13667	9.51	ppb	94
9) Chloroethane	1.79	64	9886	9.09	ppb	98
10) Dichlorofluoromethane	1.99	67	36624	9.82	ppb	92
11) Trichlorofluoromethane	2.02	101	40714	9.13	ppb	95
13) Acrolein	2.46	56	22939	106.35	ppb	96
14) Acetone	2.63	43	23346	46.39	ppb	93
15) Freon-113	2.56	151	18114	9.98	ppb	96
16) Acetonitrile	2.96	41	14889	124.49	ppb	92
18) 1,2-Dichlorotrifluoroethan	1.99	67	36624	9.82	ppb	100
19) 1,1-DCE	2.53	61	26715	9.88	ppb	92
20) t-Butanol	3.37	59	20764	133.44	ppb	94
21) Methyl Acetate	3.02	43	7535	8.90	ppb	88
22) Iodomethane	2.68	142	14870	8.17	ppb	98
23) Acrylonitrile	3.46	53	4761	10.00	ppb	93
25) Methylene chloride	3.11	84	16655	9.55	ppb	96
26) Carbon disulfide	2.74	76	21032	9.57	ppb	96
27) Methyl t-butyl ether (MtBE)	3.50	73	55621	9.56	ppb	95
28) Trans-1,2-DCE	3.47	96	17905	9.50	ppb	90
29) 3-Methylpentane	3.50	57	10514	10.71	ppb	99
31) Diisopropyl Ether	4.28	45	37552	10.35	ppb	99
32) 1,1-DCA	4.10	63	28635	10.13	ppb	# 94
34) Ethyl tert Butyl Ether	4.80	59	46342	9.94	ppb	99
35) Methylcyclopentane	4.77	56	152	-0.55	ppb	100

(#) = qualifier out of range (m) = manual integration

Data File : M:\MAX\DATA\211015\1026M25.D
 Acq On : 26 Oct 21 20:30
 Sample : 211026B CCV 10ug/L
 Misc : IS&S 8/4/21

Vial: 25
 Operator: LP, DG, CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 27 7:38 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 14:01:48 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
36) MEK (2-Butanone)	5.02	43	26949	51.22	ppb	# 90
37) Cis-1,2-DCE	4.95	96	19705	9.44	ppb	97
38) 2,2-Dichloropropane	4.93	77	32994	9.10	ppb	98
39) Chloroform	5.39	83	39095	10.65	ppb	86
40) Bromochloromethane	5.25	130	15194	9.27	ppb	92
42) 1,1,1-TCA	5.57	97	44364	10.29	ppb	90
43) Cyclohexane	5.62	41	12836	10.41	ppb	# 75
44) 1,1-Dichloropropene	5.79	75	22986	9.83	ppb	96
45) 2,2,4-Trimethylpentane	6.15	57	29028	9.57	ppb	86
47) Carbon Tetrachloride	5.77	117	40570	10.01	ppb	90
48) Tert Amyl Methyl Ether	6.22	73	43951	9.56	ppb	98
49) 1,2-DCA	6.07	62	35268	9.72	ppb	98
50) Benzene	6.03	78	63603	9.40	ppb	99
51) TCE	6.78	95	19974	9.22	ppb	81
52) 2-Pentanone	7.04	43	110476	125.61	ppb	96
53) 1,2-Dichloropropane	7.03	63	7270	9.66	ppb	94
54) Bromodichloromethane	7.34	83	30118	9.91	ppb	100
55) Methyl Cyclohexane	6.97	83	21880	9.40	ppb	77
56) Dibromomethane	7.15	93	11854	8.97	ppb	93
57) MIBK (methyl isobutyl ket	8.01	43	57899	51.47	ppb	97
58) 1-Bromo-2-chloroethane	7.65	144	3990	9.39	ppb	# 69
60) Cis-1,3-Dichloropropene	7.82	75	27060	9.94	ppb	94
61) Toluene	8.14	91	74751	9.55	ppb	95
62) Trans-1,3-Dichloropropene	8.40	75	25875	9.58	ppb	100
63) 1,1,2-TCA	8.58	83	11165	9.20	ppb	87
64) 2-Hexanone	8.86	43	38950	51.20	ppb	89
67) 1,2-EDB	9.06	107	16589	9.14	ppb	96
68) Tetrachloroethene	8.69	164	14944	8.08	ppb	90
69) 1-Chlorohexane	9.56	91	11399	8.35	ppb	97
70) 1,1,1,2-Tetrachloroethane	9.65	131	27800	10.87	ppb	96
71) m&p-Xylene	9.79	106	79546	20.46	ppb	95
72) o-Xylene	10.19	106	38623	9.47	ppb	90
73) Styrene	10.20	104	61999	10.10	ppb	96
75) 1,3-Dichloropropane	8.74	76	25465	9.54	ppb	89
76) Dibromochloromethane	8.96	129	26213	9.82	ppb	97
77) Chlorobenzene	9.56	112	59728	10.02	ppb	91
78) Ethylbenzene	9.68	91	94597	10.02	ppb	99
79) Bromoform	10.37	173	21361	9.64	ppb	90
81) Isopropylbenzene	10.56	105	104145	9.80	ppb	98
82) 1,1,2,2-Tetrachloroethane	10.87	83	16957	9.30	ppb	# 94
83) 1,2,3-Trichloropropane	10.90	110	8957	9.83	ppb	90
84) t-1,4-Dichloro-2-Butene	10.93	53	4864	10.48	ppb	# 54

(#) = qualifier out of range (m) = manual integration

Data File : M:\MAX\DATA\211015\1026M25.D
 Acq On : 26 Oct 21 20:30
 Sample : 211026B CCV 10ug/L
 Misc : IS&S 8/4/21

Vial: 25
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 27 7:38 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 14:01:48 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
85) Bromobenzene	10.84	156	33801	9.72	ppb	91
86) n-Propylbenzene	10.97	91	102142	9.73	ppb	93
87) 4-Ethyltoluene	11.08	105	97233	10.04	ppb	92
88) 2-Chlorotoluene	11.04	91	81407	9.79	ppb	93
89) 1,3,5-Trimethylbenzene	11.14	105	91867	10.13	ppb	98
90) 4-Chlorotoluene	11.15	91	79568	9.63	ppb	97
91) Tert-Butylbenzene	11.47	119	53208	10.63	ppb	97
92) 1,2,4-Trimethylbenzene	11.51	105	87930	10.24	ppb	94
93) Sec-Butylbenzene	11.68	105	100516	10.50	ppb	94
94) p-Isopropyltoluene	11.83	119	94043	10.16	ppb	99
95) Benzyl Chloride	12.01	91	17253	7.87	ppb	99
96) 1,3-DCB	11.78	146	59463	9.82	ppb	98
97) 1,4-DCB	11.87	146	60321	9.78	ppb	94
98) n-Butylbenzene	12.24	91	55543	9.03	ppb	98
99) 1,2-DCB	12.24	146	57208	9.65	ppb	98
100) Hexachloroethane	12.48	117	16682	10.75	ppb	91
101) 1,2-Dibromo-3-chloropropan	13.02	75	4271	8.42	ppb #	87
102) 1,2,4-Trichlorobenzene	13.84	180	19616	8.56	ppb	86
103) Hexachlorobutadiene	14.02	225	22274	8.90	ppb	94
104) Naphthalene	14.08	128	34929	8.29	ppb #	92
105) 1,2,3-Trichlorobenzene	14.32	180	24336	8.37	ppb	85

Quantitation Report


Data File : M:\MAX\DATA\211015\1026M25.D
Acq On : 26 Oct 21 20:30
Sample : 211026B CCV 10ug/L
Misc : IS&S 8/4/21

Vial: 25
Operator: LP,DG,CH
Inst : Max
Multiplr: 1.00

Quant Time: Oct 27 7:38 2021

Quant Results File: M1015W.RES

Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
Title : METHOD 8260B
Last Update : Sat Oct 16 14:01:48 2021
Response via : Initial Calibration

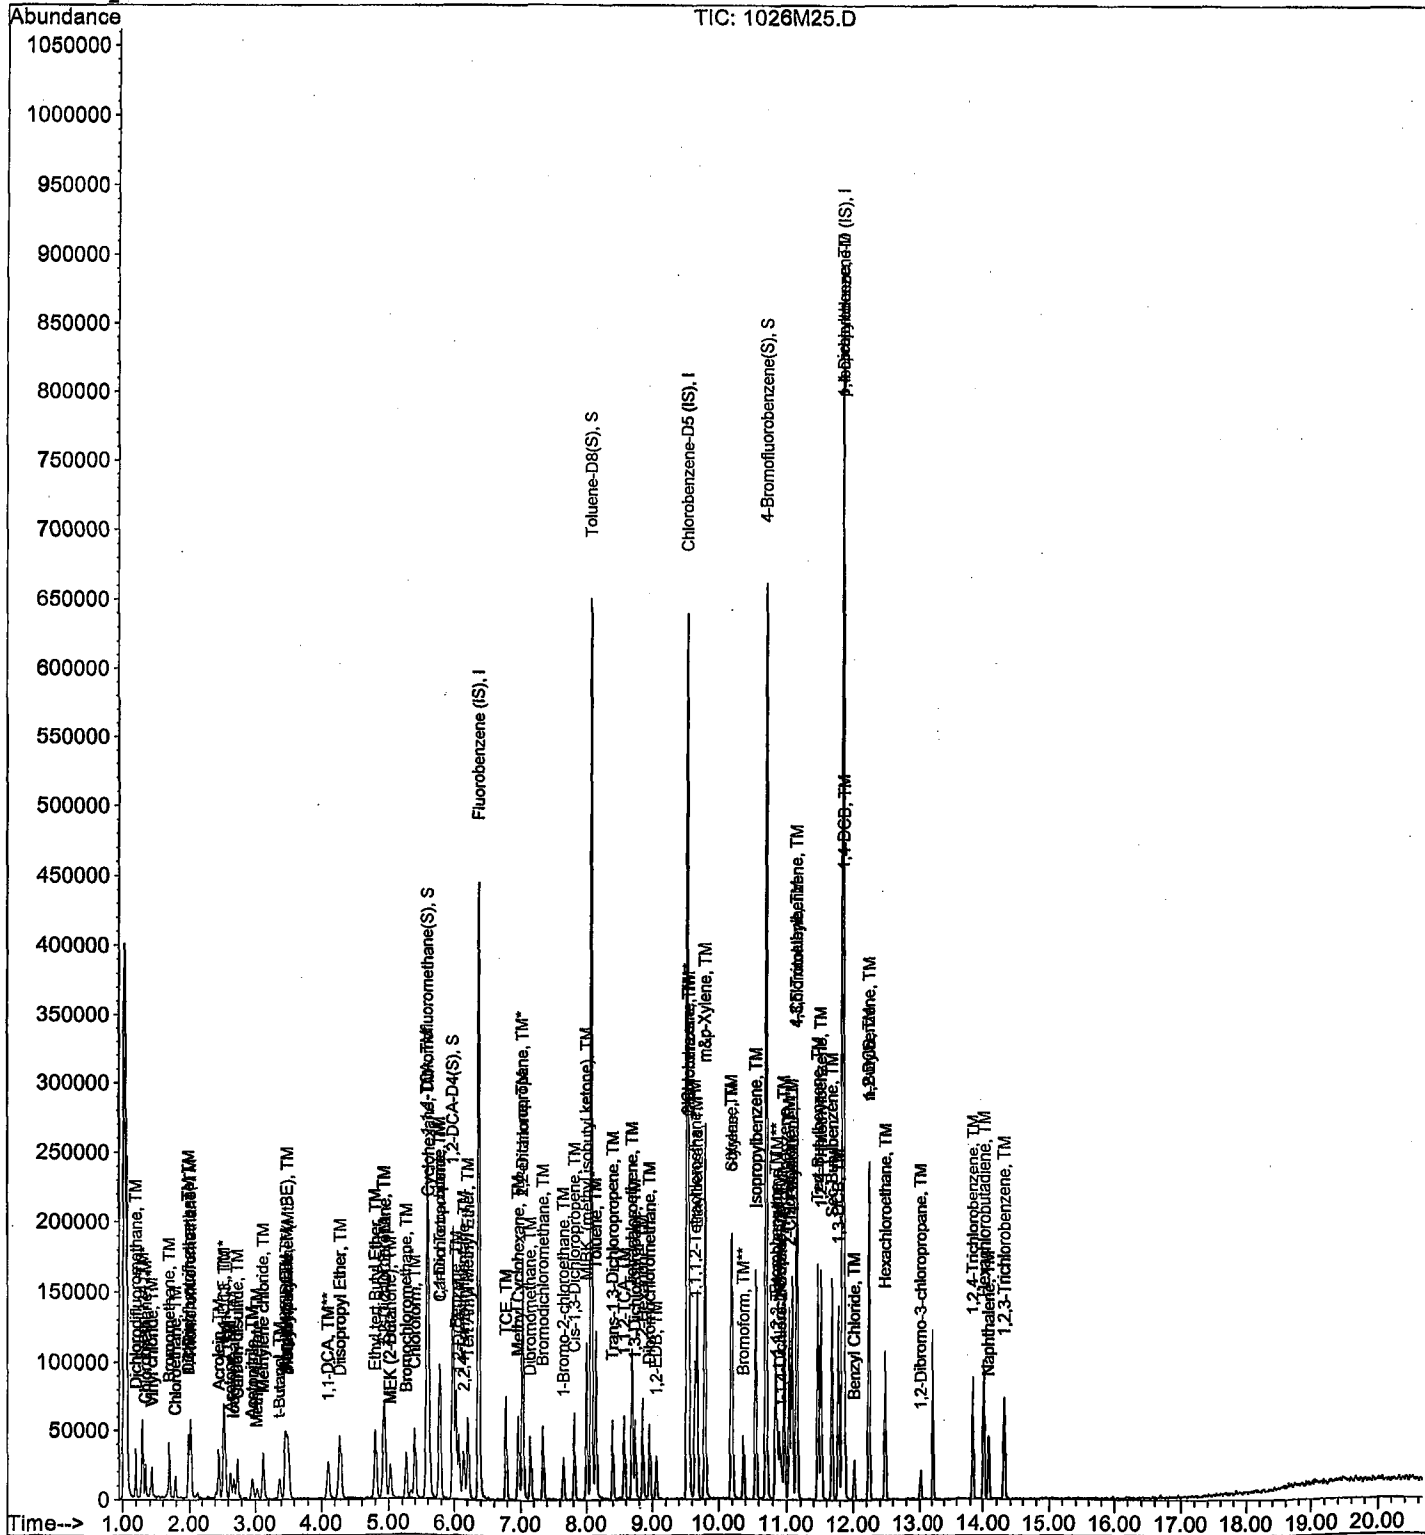

VOLATILE ORGANIC ANALYSIS BY
EPA METHOD 8260B

Form 7

Ending Continuing Calibration

Lab Name: APPL, Inc.
Case No: _____
Matrix: Water

SDG No: _____
Date Analyzed: 10/27/2021
Instrument: Max
Initial Cal. Date: 10/15/2021
Data File: 1026M45.D

		Compound	MEAN	CCRF	%D	%Drift
1	I	Fluorobenzene (IS)	ISTD			I
2	TM	Chlorotrifluoroethene	0.0000	0.0154	0.00	TM
3	TM	Dichlorodifluoromethane	0.1497	0.1189	21	TM
4	TM	Freon 114	0.0839	0.0852	1.6	TM
5	TM**	Chloromethane	0.0893	0.0782	12	TM**
6	TM*	Vinyl chloride	0.1101	0.0869	21	TM*
7	TM	2-Chloro-1,1,1-trifluoroethane	0.0000	0.0029	0.00	TM
8	TM	Bromomethane	0.0931	0.0867	6.8	TM
9	TML	Chloroethane	0.0844	0.0558	34	TML 19
10	TM	Dichlorofluoromethane	0.2416	0.2278	5.7	TM
11	TM	Trichlorofluoromethane	0.2889	0.2462	15	TM
12	TMQ	Acrolein	0.0145	0.0102	29	TMQ 27
13	TM	Acetone	0.0326	0.0266	18	TM
14	TM	Freon-113	0.1176	0.1228	4.4	TM
15	TM	Acetonitrile	0.0077	0.0071	8.7	TM
16	TML	2-propanol	0.0000	0.0009	0.00	TML
17	TM	1,2-Dichlorotrifluoroethane	0.2416	0.2278	5.7	TM
18	TM*	1,1-DCE	0.1751	0.1633	6.7	TM*
19	TMQ	t-Butanol	0.0101	0.0105	3.2	TMQ 3.4
20	TMQ	Methyl Acetate	0.0528	0.0490	7.3	TMQ 11
21	TML	Iodomethane	0.1096	0.1089	0.63	TML 9.2
22	TML	Acrylonitrile	0.0252	0.0294	17	TML 4.8
23	TM	2-Methylpentane	0.0000	0.0003	0.00	TM
24	TM	Methylene chloride	0.1130	0.1198	6.0	TM
25	TM	Carbon disulfide	0.1424	0.1378	3.3	TM
26	TM	Methyl t-butyl ether (MtBE)	0.3769	0.3545	5.9	TM
27	TM	Trans-1,2-DCE	0.1221	0.1037	15	TM
28	TML	3-Methylpentane	0.0702	0.0601	14	TML 6.0
29	TM	Hexane	0.0000	0.0001	0.00	TM
30	TM	Diisopropyl Ether	0.2351	0.2526	7.4	TM
31	TM**	1,1-DCA	0.1831	0.1896	3.5	TM**
32	TM	Ethyl tert Butyl Ether	0.3021	0.3159	4.6	TM
33	TML	Methylcyclopentane	0.0160	0.0115	28	TML 13
34	TM	MEK (2-Butanone)	0.0341	0.0315	7.5	TM
35	TM	Cis-1,2-DCE	0.1352	0.1316	2.6	TM
36	TM	2,2-Dichloropropane	0.2349	0.1745	26	TM
37	TM*	Chloroform	0.2377	0.2623	10	TM*
38	TML	Bromochloromethane	0.1040	0.0980	5.7	TML 7.7
39	S	Dibromofluoromethane(S)	0.3105	0.3192	2.8	S
40	TM	1,1,1-TCA	0.2791	0.2862	2.5	TM

Average

9.3

VOLATILE ORGANIC ANALYSIS BY
EPA METHOD 8260B

Form 7

Ending Continuing Calibration

Lab Name: APPL, Inc.
Case No: _____
Matrix: Water

SDG No: _____
Date Analyzed: 10/27/2021
Instrument: Max
Cal. Date: 10/15/2021
Data File: 1026M45.D

		Compound	MEAN	CCRF	%D	%Drift
41	TM	Cyclohexane	0.0798	0.0810	1.4	TM
42	TM	1,1-Dichloropropene	0.1514	0.1610	6.3	TM
43	TM	2,2,4-Trimethylpentane	0.1964	0.1759	10	TM
44	S	1,2-DCA-D4(S)	0.2166	0.2176	0.49	S
45	TM	Carbon Tetrachloride	0.2625	0.2521	3.9	TM
46	TM	Tert Amyl Methyl Ether	0.2978	0.2948	1.0	TM
47	TM	1,2-DCA	0.2350	0.2280	3.0	TM
48	TM	Benzene	0.4384	0.4232	3.5	TM
49	TM	TCE	0.1404	0.1384	1.4	TM
50	TM	2-Pentanone	0.0570	0.0541	5.1	TM
51	TM*L	1,2-Dichloropropane	0.0476	0.0524	10	TM*L 8.0
52	TM	Bromodichloromethane	0.1968	0.2084	5.9	TM
53	TML	Methyl Cyclohexane	0.1542	0.1450	5.9	TML 3.9
54	TM	Dibromomethane	0.0856	0.0756	12	TM
55	TM	MIBK (methyl isobutyl ketone)	0.0729	0.0701	3.7	TM
56	TML	1-Bromo-2-chloroethane	0.0245	0.0267	9.1	TML 2.9
57	TM	2-Chloroethyl vinyl ether	0.0000	0.0000	0.00	TM
58	TM	Cis-1,3-Dichloropropene	0.1763	0.1768	0.28	TM
59	TM*	Toluene	0.5070	0.5036	0.66	TM*
60	TM	Trans-1,3-Dichloropropene	0.1749	0.1755	0.36	TM
61	TM	1,1,2-TCA	0.0786	0.0771	1.9	TM
62	TM	2-Hexanone	0.0493	0.0459	6.7	TM
63	I	Chlorobenzene-D5 (IS)	ISTD			I
64	S	Toluene-D8(S)	1.149	1.159	0.83	S
65	TM	1,2-EDB	0.1319	0.1236	6.3	TM
66	TML	Tetrachloroethene	0.2207	0.1250	43	TML 4.8
67	TM	1-Chlorohexane	0.0992	0.0980	1.3	TM
68	TM	1,1,1,2-Tetrachloroethane	0.1860	0.1957	5.2	TM
69	TM	m&p-Xylene	0.2826	0.2930	3.7	TM
70	TM	o-Xylene	0.2964	0.2859	3.5	TM
71	TM	Styrene	0.4463	0.4515	1.2	TM
72	S	4-Bromofluorobenzene(S)	0.4641	0.4666	0.54	S
73	TM	1,3-Dichloropropane	0.1940	0.1852	4.5	TM
74	TM	Dibromochloromethane	0.1941	0.1901	2.0	TM
75	TM**	Chlorobenzene	0.4334	0.4401	1.6	TM**
76	TM*	Ethylbenzene	0.6860	0.6813	0.68	TM*
77	TM**	Bromoform	0.1611	0.1526	5.3	TM**
78	I	1,4-Dichlorobenzene-D (IS)	ISTD			I
79	TM	Isopropylbenzene	1.166	1.163	0.26	TM
80	TM**	1,1,2,2-Tetrachloroethane	0.2001	0.1823	8.9	TM**

Average

4.8

VOLATILE ORGANIC ANALYSIS BY
EPA METHOD 8260B

Form 7

Ending Continuing Calibration

Lab Name: APPL, Inc.
Case No: _____
Matrix: Water

SDG No: _____
Date Analyzed: 10/27/2021
Instrument: Max
Cal. Date: 10/15/2021
Data File: 1026M45.D

		Compound	MEAN	CCRF	%D	%Drift	
81	TM	1,2,3-Trichloropropane	0.1000	0.0918	8.2	TM	
82	TML	t-1,4-Dichloro-2-Butene	0.0601	0.0444	26	TML	12
83	TM	Bromobenzene	0.3816	0.3844	0.73	TM	
84	TM	n-Propylbenzene	1.151	1.195	3.7	TM	
85	TM	4-Ethyltoluene	1.063	1.111	4.5	TM	
86	TM	2-Chlorotoluene	0.9129	0.8979	1.6	TM	
87	TM	1,3,5-Trimethylbenzene	0.9948	0.9968	0.20	TM	
88	TM	4-Chlorotoluene	0.9068	0.9134	0.73	TM	
89	TM	Tert-Butylbenzene	0.5492	0.5888	7.2	TM	
90	TM	1,2,4-Trimethylbenzene	0.9425	1.010	7.1	TM	
91	TM	Sec-Butylbenzene	1.051	1.135	8.0	TM	
92	TM	p-Isopropyltoluene	1.016	1.081	6.4	TM	
93	TM	Benzyl Chloride	0.2406	0.1364	43	TM	
94	TM	1,3-DCB	0.6644	0.8828	2.8	TM	
95	TM	1,4-DCB	0.6767	0.8827	0.89	TM	
96	TML	n-Butylbenzene	0.5721	0.5954	4.1	TML	12
97	TM	1,2-DCB	0.6504	0.6446	0.89	TM	
98	TM	Hexachloroethane	0.1703	0.1708	0.31	TM	
99	TML	1,2-Dibromo-3-chloropropane	0.0437	0.0445	1.7	TML	20
100	TML	1,2,4-Trichlorobenzene	0.1936	0.1929	0.38	TML	21
101	TML	Hexachlorobutadiene	0.2401	0.2387	0.58	TML	13
102	TMQ	Naphthalene	0.4088	0.3791	7.3	TMQ	18
103	TML	1,2,3-Trichlorobenzene	0.2371	0.2631	11	TML	17
104							
105							
106							
107							
108							
109							
110							
111							
112							
113							
114							
115							
116							
117							
118							
119							
120							

Average

6.4

Data File : M:\MAX\DATA\211015\1026M45.D
 Acq On : 27 Oct 21 5:55
 Sample : Ending CCV 10ug/L 10/26/21
 Misc : IS&S 8/4/21

Vial: 45
 Operator: LP, DG, CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 27 7:38 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 14:01:48 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.37	96	387172	25.00	ppb	0.03
65) Chlorobenzene-D5 (IS)	9.52	117	351019	25.00	ppb	0.03
80) 1,4-Dichlorobenzene-D (IS)	11.84	152	224090	25.00	ppb	0.02

System Monitoring Compounds

41) Dibromofluoromethane (S)	5.59	111	123594	25.70	ppb	0.03
Spiked Amount	25.000		Recovery	= 102.812%		
46) 1,2-DCA-D4 (S)	5.98	65	84256	25.12	ppb	0.03
Spiked Amount	25.000		Recovery	= 100.488%		
66) Toluene-D8 (S)	8.08	98	406676	25.21	ppb	0.03
Spiked Amount	25.000		Recovery	= 100.828%		
74) 4-Bromofluorobenzene (S)	10.70	95	163775	25.13	ppb	0.02
Spiked Amount	25.000		Recovery	= 100.536%		

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Dichlorodifluoromethane	1.19	85	18416	7.94	ppb	98
4) Freon 114	1.30	85	13197	10.16	ppb	86
5) Chloromethane	1.34	50	12114	8.76	ppb	99
6) Vinyl chloride	1.43	62	13451	7.89	ppb	100
8) Bromomethane	1.69	94	13434	9.32	ppb	95
9) Chloroethane	1.79	64	8643	8.07	ppb	96
10) Dichlorofluoromethane	1.99	67	35275	9.43	ppb	98
11) Trichlorofluoromethane	2.02	101	38134	8.52	ppb	90
13) Acrolein	2.45	56	19792	91.65	ppb	96
14) Acetone	2.63	43	20595	40.80	ppb	95
15) Freon-113	2.55	151	19016	10.44	ppb	89
16) Acetonitrile	2.95	41	13697	114.18	ppb	90
18) 1,2-Dichlorotrifluoroethan	1.99	67	35275	9.43	ppb	100
19) 1,1-DCE	2.53	61	25296	9.33	ppb	92
20) t-Butanol	3.36	59	20240	129.25	ppb	94
21) Methyl Acetate	3.02	43	7582	8.93	ppb	99
22) Iodomethane	2.68	142	16869	9.08	ppb	97
23) Acrylonitrile	3.47	53	4550	9.52	ppb	# 58
25) Methylene chloride	3.11	84	18553	10.60	ppb	87
26) Carbon disulfide	2.73	76	21336	9.67	ppb	95
27) Methyl t-butyl ether (MtBE)	3.50	73	54908	9.41	ppb	95
28) Trans-1,2-DCE	3.46	96	16061	8.50	ppb	93
29) 3-Methylpentane	3.50	57	9313	9.40	ppb	90
31) Diisopropyl Ether	4.27	45	39113	10.74	ppb	98
32) 1,1-DCA	4.09	63	29360	10.35	ppb	# 92
34) Ethyl tert Butyl Ether	4.80	59	48925	10.46	ppb	92
35) Methylcyclopentane	4.79	56	1776	8.65	ppb	100

(#) = qualifier out of range (m) = manual integration

Data File : M:\MAX\DATA\211015\1026M45.D
 Acq On : 27 Oct 21 5:55
 Sample : Ending CCV 10ug/L 10/26/21
 Misc : IS&S 8/4/21

Vial: 45
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 27 7:38 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 14:01:48 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
36) MEK (2-Butanone)	5.02	43	24415	46.26	ppb	91
37) Cis-1,2-DCE	4.94	96	20386	9.74	ppb	97
38) 2,2-Dichloropropane	4.93	77	27018	7.43	ppb #	86
39) Chloroform	5.39	83	40623	11.04	ppb	98
40) Bromochloromethane	5.25	130	15179	9.23	ppb #	84
42) 1,1,1-TCA	5.57	97	44321	10.25	ppb	94
43) Cyclohexane	5.61	41	12538	10.14	ppb	82
44) 1,1-Dichloropropene	5.78	75	24928	10.63	ppb	93
45) 2,2,4-Trimethylpentane	6.15	57	27244	8.96	ppb	85
47) Carbon Tetrachloride	5.77	117	39049	9.61	ppb	84
48) Tert Amyl Methyl Ether	6.22	73	45650	9.90	ppb	98
49) 1,2-DCA	6.07	62	35306	9.70	ppb #	92
50) Benzene	6.02	78	65536	9.65	ppb	96
51) TCE	6.78	95	21430	9.86	ppb #	83
52) 2-Pentanone	7.03	43	104696	118.68	ppb	98
53) 1,2-Dichloropropane	7.02	63	8121	10.80	ppb	97
54) Bromodichloromethane	7.34	83	32272	10.59	ppb	93
55) Methyl Cyclohexane	6.97	83	22460	9.61	ppb	87
56) Dibromomethane	7.15	93	11712	8.83	ppb	93
57) MIBK (methyl isobutyl ket)	8.00	43	54297	48.13	ppb	97
58) 1-Bromo-2-chloroethane	7.65	144	4142	9.71	ppb	86
60) Cis-1,3-Dichloropropene	7.81	75	27386	10.03	ppb	90
61) Toluene	8.14	91	77994	9.93	ppb	97
62) Trans-1,3-Dichloropropene	8.39	75	27178	10.04	ppb	99
63) 1,1,2-TCA	8.57	83	11941	9.81	ppb	93
64) 2-Hexanone	8.85	43	35577	46.63	ppb	95
67) 1,2-EDB	9.05	107	17359	9.37	ppb	88
68) Tetrachloroethene	8.69	164	17552	9.52	ppb	84
69) 1-Chlorohexane	9.55	91	13753	9.87	ppb	91
70) 1,1,1,2-Tetrachloroethane	9.64	131	27480	10.52	ppb	96
71) m&p-Xylene	9.79	106	82282	20.74	ppb	98
72) o-Xylene	10.18	106	40139	9.65	ppb	94
73) Styrene	10.20	104	63387	10.12	ppb #	96
75) 1,3-Dichloropropane	8.73	76	25999	9.55	ppb	98
76) Dibromochloromethane	8.96	129	26693	9.80	ppb	97
77) Chlorobenzene	9.55	112	61798	10.16	ppb	99
78) Ethylbenzene	9.67	91	95663	9.93	ppb	95
79) Bromoform	10.37	173	21423	9.47	ppb	99
81) Isopropylbenzene	10.55	105	104225	9.97	ppb	96
82) 1,1,2,2-Tetrachloroethane	10.87	83	16338	9.11	ppb	96
83) 1,2,3-Trichloropropane	10.89	110	8233	9.18	ppb	87
84) t-1,4-Dichloro-2-Butene	10.92	53	3982	8.76	ppb #	54

(#) = qualifier out of range (m) = manual integration

Data File : M:\MAX\DATA\211015\1026M45.D
 Acq On : 27 Oct 21 5:55
 Sample : Ending CCV 10ug/L 10/26/21
 Misc : IS&S 8/4/21

Vial: 45
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 27 7:38 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 14:01:48 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Compound	R.T.	QIion	Response	Conc	Unit	Qvalue
85) Bromobenzene	10.84	156	34459	10.07	ppb	97
86) n-Propylbenzene	10.97	91	107071	10.37	ppb	96
87) 4-Ethyltoluene	11.08	105	99548	10.45	ppb	97
88) 2-Chlorotoluene	11.04	91	80484	9.84	ppb	93
89) 1,3,5-Trimethylbenzene	11.14	105	89346	10.02	ppb	97
90) 4-Chlorotoluene	11.15	91	81873	10.07	ppb	97
91) Tert-Butylbenzene	11.46	119	52776	10.72	ppb	100
92) 1,2,4-Trimethylbenzene	11.51	105	90510	10.71	ppb	100
93) Sec-Butylbenzene	11.68	105	101730	10.80	ppb	98
94) p-Isopropyltoluene	11.83	119	96922	10.64	ppb	100
95) Benzyl Chloride	12.01	91	12223	5.67	ppb	96
96) 1,3-DCB	11.78	146	61205	10.28	ppb	98
97) 1,4-DCB	11.87	146	61196	10.09	ppb	94
98) n-Butylbenzene	12.24	91	53372	8.85	ppb	98
99) 1,2-DCB	12.23	146	57780	9.91	ppb	99
100) Hexachloroethane	12.48	117	15309	10.03	ppb	90
101) 1,2-Dibromo-3-chloropropan	13.02	75	3985	8.04	ppb	90
102) 1,2,4-Trichlorobenzene	13.83	180	17288	7.90	ppb	94
103) Hexachlorobutadiene	14.01	225	21400	8.72	ppb	95
104) Naphthalene	14.08	128	33985	8.21	ppb	97
105) 1,2,3-Trichlorobenzene	14.32	180	23587	8.28	ppb	91

(#) = qualifier out of range (m) = manual integration
 1026M45.D M1015W.M Wed Oct 27 07:59:18 2021

Quantitation Report


Data File : M:\MAX\DATA\211015\1026M45.D
Acq On : 27 Oct 21 5:55
Sample : Ending CCV 10ug/L 10/26/21
Misc : IS&S 8/4/21

Vial: 45
Operator: LP,DG,CH
Inst : Max
Multiplr: 1.00

Quant Time: Oct 27 7:38 2021

Quant Results File: M1015W.RES

Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
Title : METHOD 8260B
Last Update : Sat Oct 16 14:01:48 2021
Response via : Initial Calibration

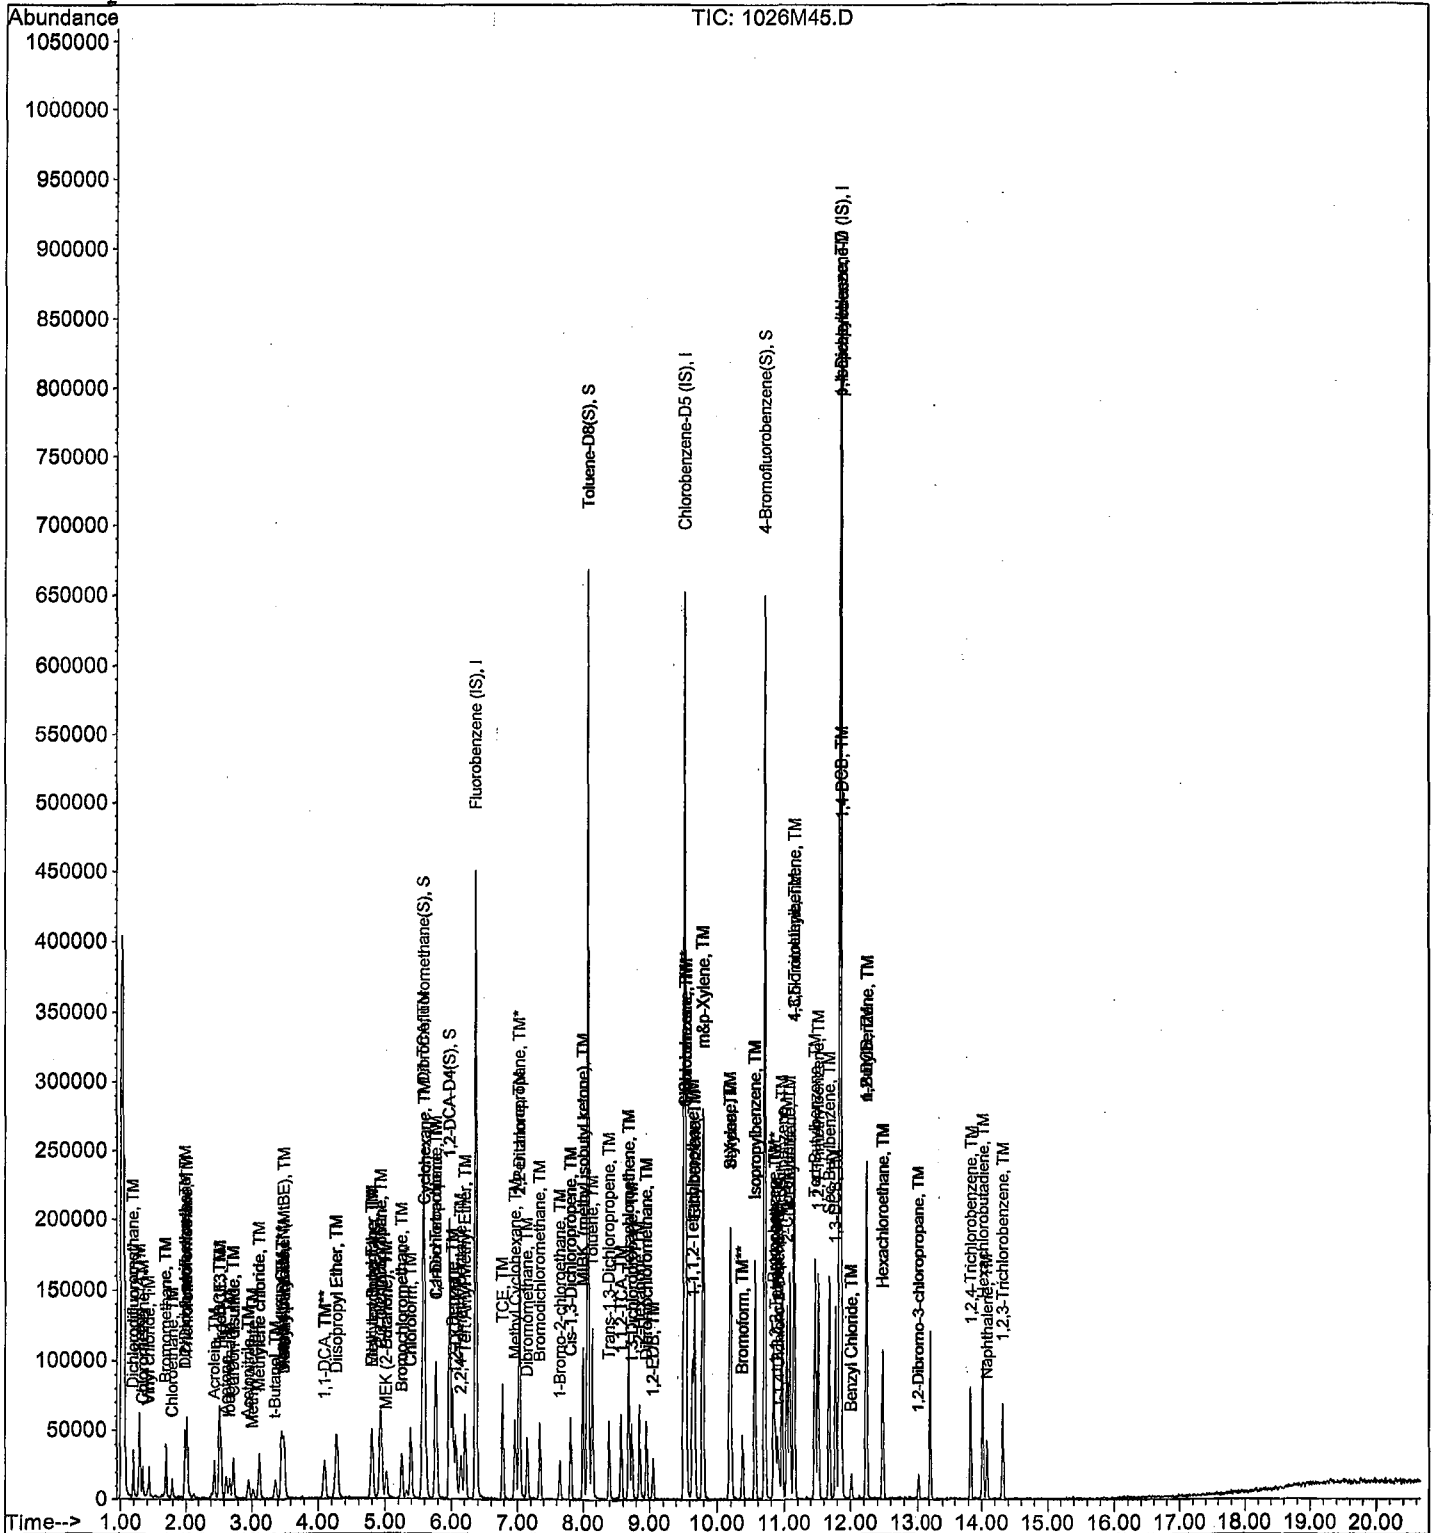

ORGANICS
Raw Data

Data File : M:\MAX\DATA\211015\1026M35.D
 Acq On : 27 Oct 21 1:13
 Sample : BA43836W01
 Misc : IS&S 8/4/21

Vial: 35
 Operator: LP, DG, CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 27 11:10 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 14:01:48 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.37	96	378804	25.00	ppb	0.03
65) Chlorobenzene-D5 (IS)	9.53	117	343273	25.00	ppb	0.03
80) 1,4-Dichlorobenzene-D (IS)	11.85	152	205124	25.00	ppb	0.03
System Monitoring Compounds						
41) Dibromofluoromethane(S)	5.59	111	122341	26.00	ppb	0.03
Spiked Amount	25.000		Recovery	=	104.020%	
46) 1,2-DCA-D4(S)	5.98	65	82080	25.01	ppb	0.03
Spiked Amount	25.000		Recovery	=	100.056%	
66) Toluene-D8(S)	8.08	98	394275	24.99	ppb	0.03
Spiked Amount	25.000		Recovery	=	99.960%	
74) 4-Bromofluorobenzene(S)	10.70	95	154312	24.22	ppb	0.03
Spiked Amount	25.000		Recovery	=	96.864%	

Target Compounds

Qvalue

Quantitation Report


Data File : M:\MAX\DATA\211015\1026M35.D
Acq On : 27 Oct 21 1:13
Sample : BA43836W01
Misc : IS&S 8/4/21

Vial: 35
Operator: LP,DG,CH
Inst : Max
Multiplr: 1.00

Quant Time: Oct 27 11:10 2021

Quant Results File: M1015W.RES

Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
Title : METHOD 8260B
Last Update : Sat Oct 16 14:01:48 2021
Response via : Initial Calibration

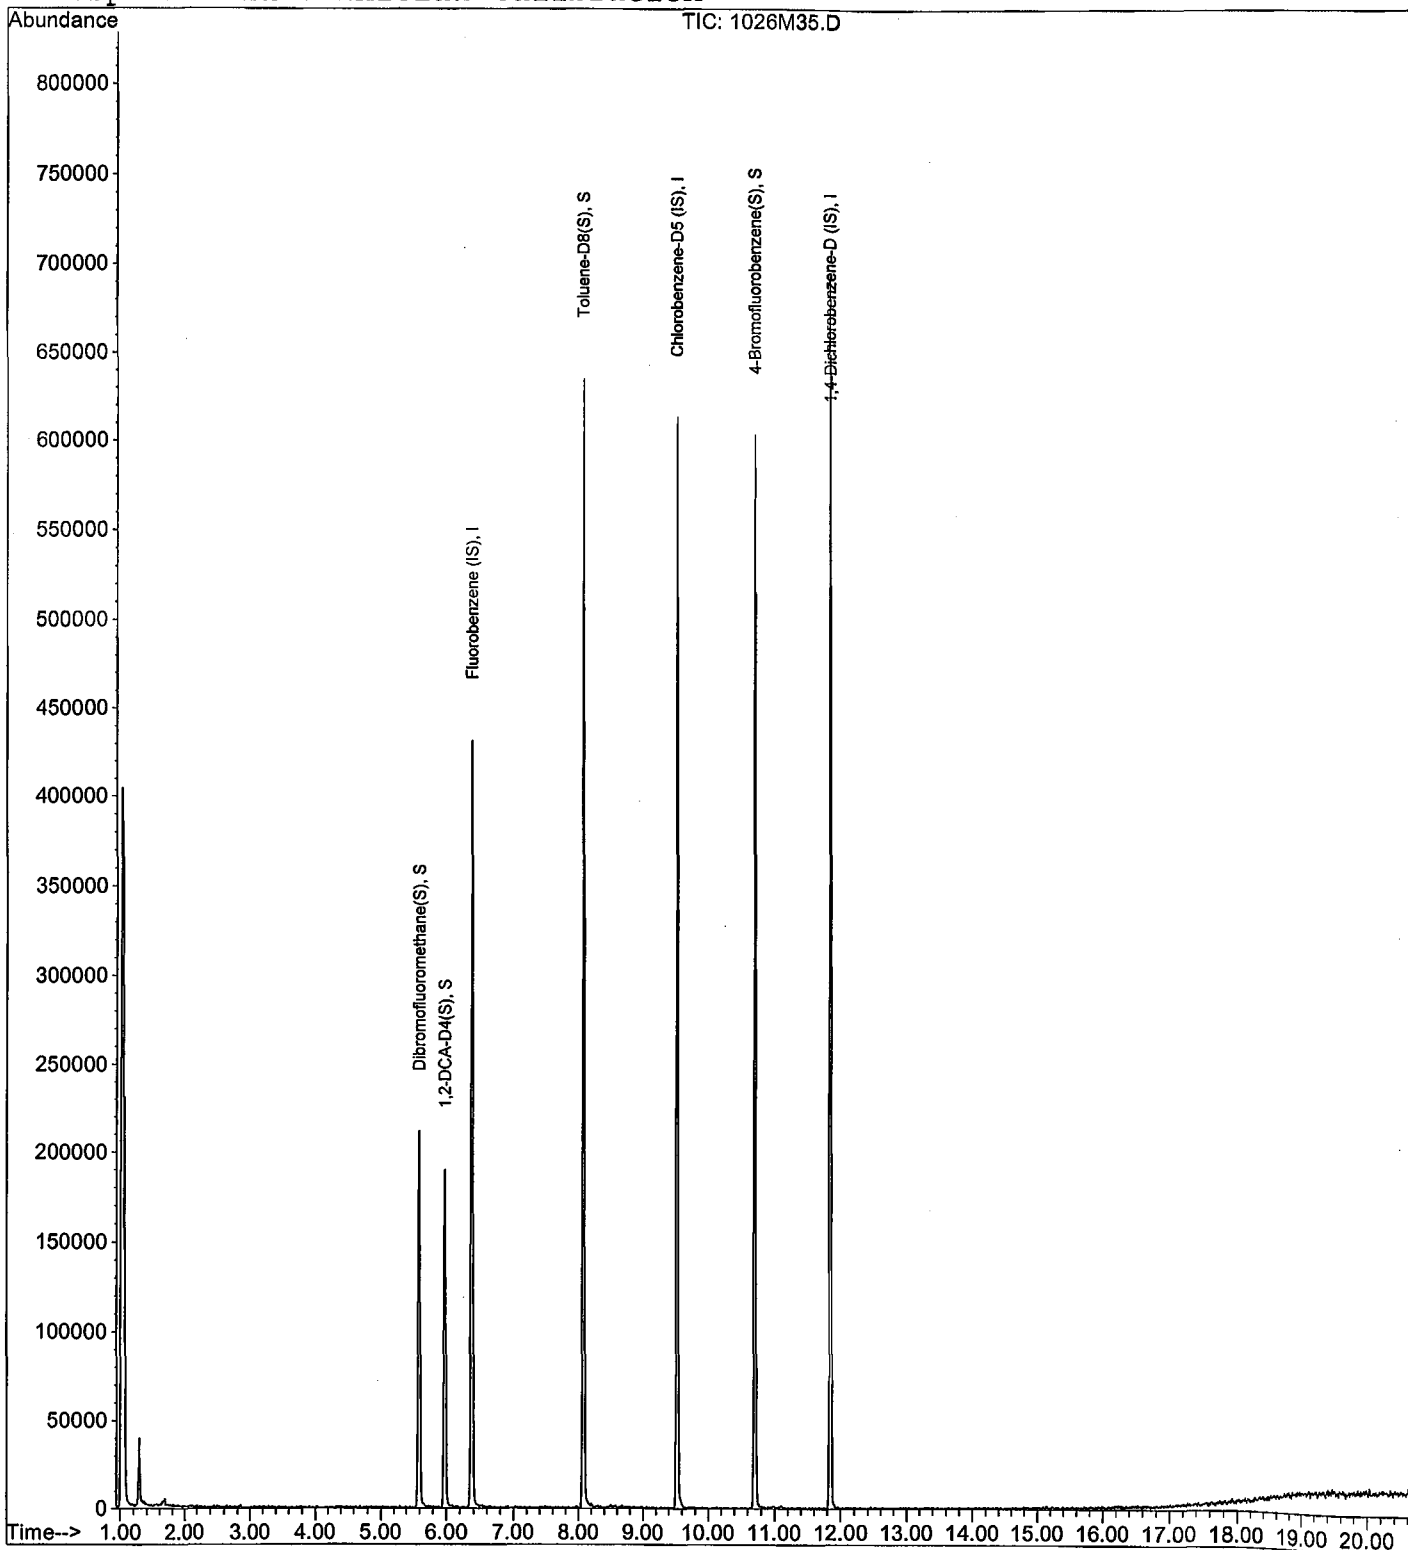

Data File : M:\MAX\DATA\211015\1026M36.D
 Acq On : 27 Oct 21 1:41
 Sample : BA43837W01
 Misc : IS&S 8/4/21

Vial: 36
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 27 11:11 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 14:01:48 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.37	96	390312	25.00	ppb	0.03
65) Chlorobenzene-D5 (IS)	9.53	117	341211	25.00	ppb	0.03
80) 1,4-Dichlorobenzene-D (IS)	11.84	152	210844	25.00	ppb	0.02
System Monitoring Compounds						
41) Dibromofluoromethane(S)	5.59	111	121910	25.15	ppb	0.03
Spiked Amount						
			Recovery	=	100.596%	
46) 1,2-DCA-D4(S)	5.98	65	82168	24.30	ppb	0.03
Spiked Amount						
			Recovery	=	97.212%	
66) Toluene-D8(S)	8.08	98	401693	25.61	ppb	0.03
Spiked Amount						
			Recovery	=	102.456%	
74) 4-Bromofluorobenzene(S)	10.70	95	152105	24.01	ppb	0.03
Spiked Amount						
			Recovery	=	96.056%	

Target Compounds

Qvalue

Quantitation Report


Data File : M:\MAX\DATA\211015\1026M36.D
Acq On : 27 Oct 21 1:41
Sample : BA43837W01
Misc : IS&S 8/4/21

Vial: 36
Operator: LP, DG, CH
Inst : Max
Multiplr: 1.00

Quant Time: Oct 27 11:11 2021

Quant Results File: M1015W.RES

Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
Title : METHOD 8260B
Last Update : Sat Oct 16 14:01:48 2021
Response via : Initial Calibration

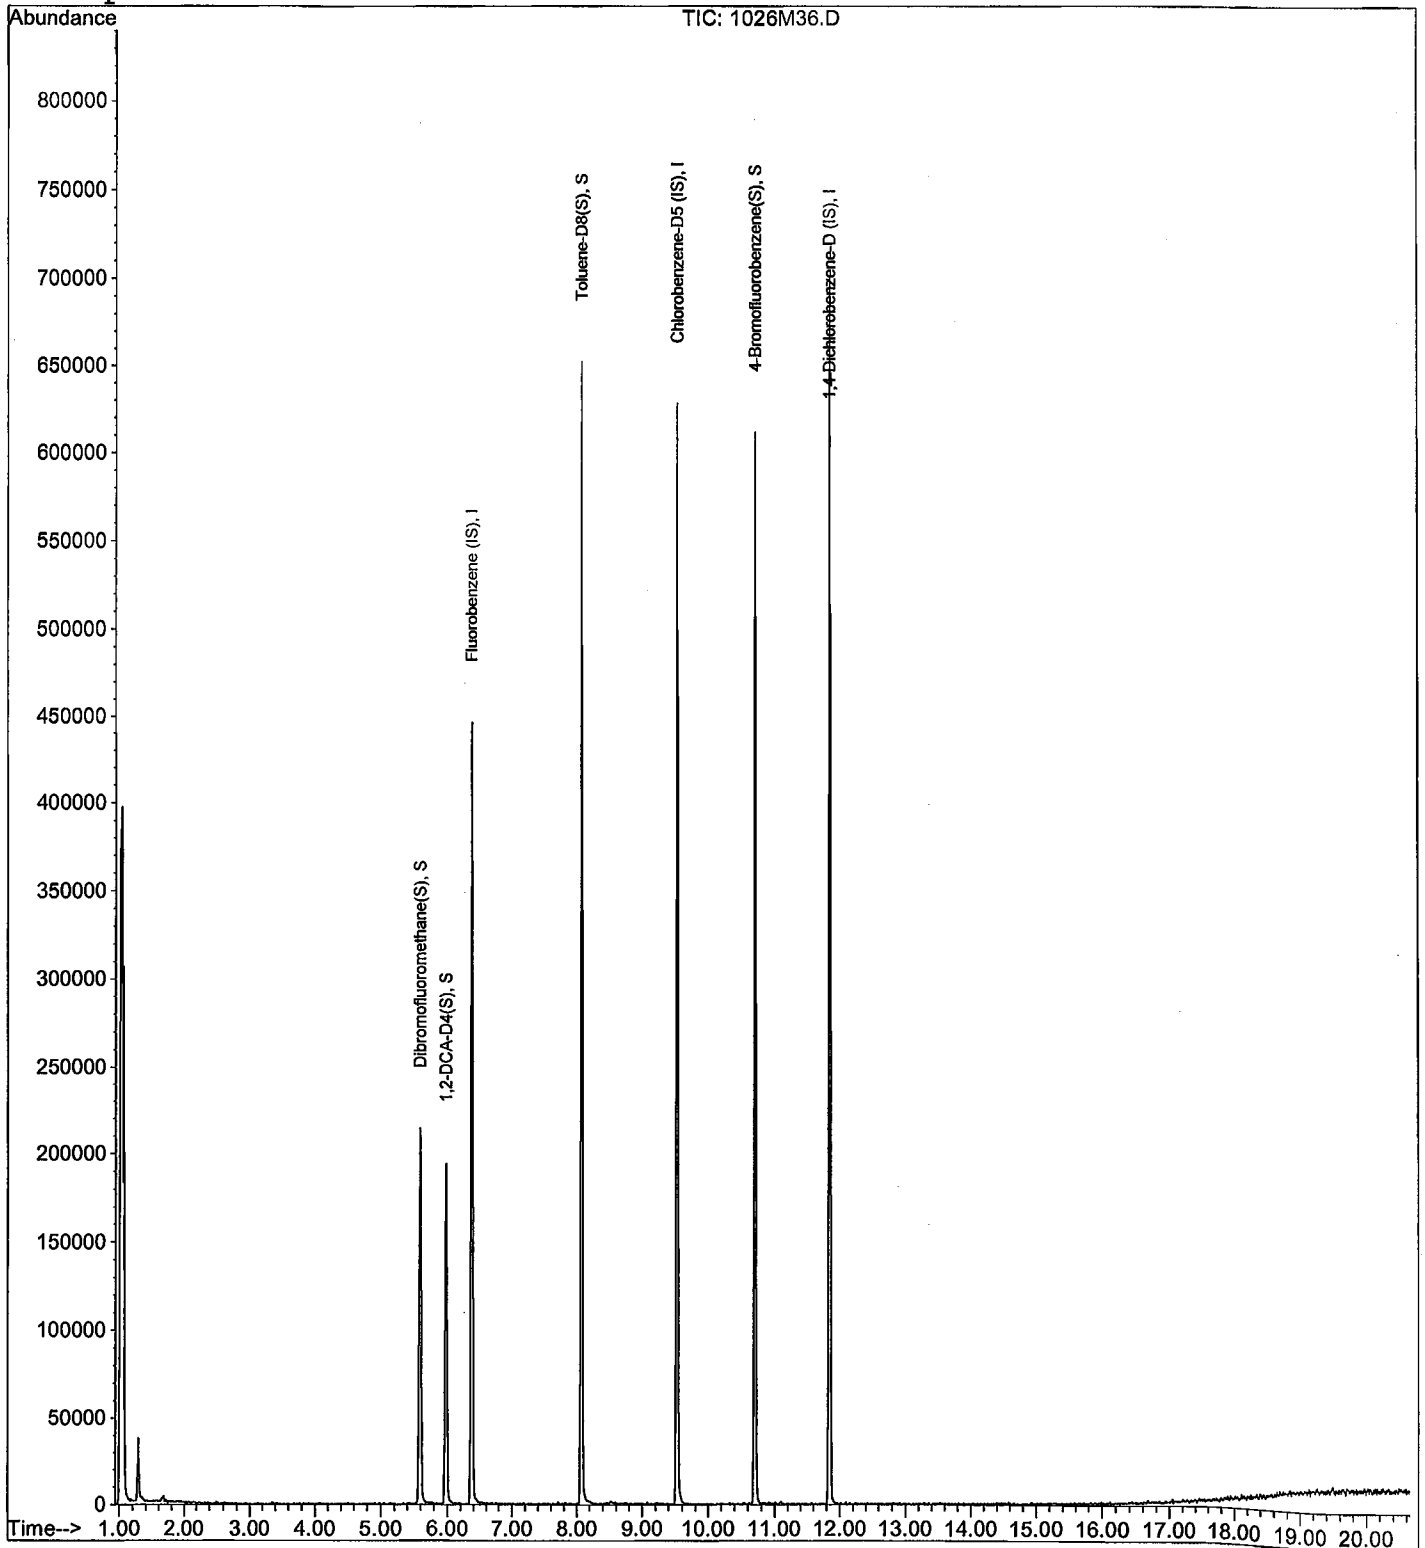

Data File : M:\MAX\DATA\211015\1026M31.D
 Acq On : 26 Oct 21 23:20
 Sample : 211026B BLK
 Misc : IS&S 8/4/21

Vial: 31
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 27 8:05 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 14:01:48 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.37	96	396235	25.00	ppb	0.03
65) Chlorobenzene-D5 (IS)	9.53	117	350438	25.00	ppb	0.03
80) 1,4-Dichlorobenzene-D (IS)	11.85	152	212898	25.00	ppb	0.03
System Monitoring Compounds						
41) Dibromofluoromethane (S)	5.59	111	122793	24.95	ppb	0.03
Spiked Amount	25.000		Recovery	=	99.808%	
46) 1,2-DCA-D4 (S)	5.98	65	85552	24.93	ppb	0.03
Spiked Amount	25.000		Recovery	=	99.700%	
66) Toluene-D8 (S)	8.08	98	398165	24.72	ppb	0.03
Spiked Amount	25.000		Recovery	=	98.880%	
74) 4-Bromofluorobenzene (S)	10.70	95	162293	24.95	ppb	0.03
Spiked Amount	25.000		Recovery	=	99.792%	

Target Compounds

Qvalue

(#) = qualifier out of range (m) = manual integration

Quantitation Report


Data File : M:\MAX\DATA\211015\1026M31.D
Acq On : 26 Oct 21 23:20
Sample : 211026B BLK
Misc : IS&S 8/4/21

Vial: 31
Operator: LP, DG, CH
Inst : Max
Multiplr: 1.00

Quant Time: Oct 27 8:05 2021

Quant Results File: M1015W.RES

Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
Title : METHOD 8260B
Last Update : Sat Oct 16 14:01:48 2021
Response via : Initial Calibration

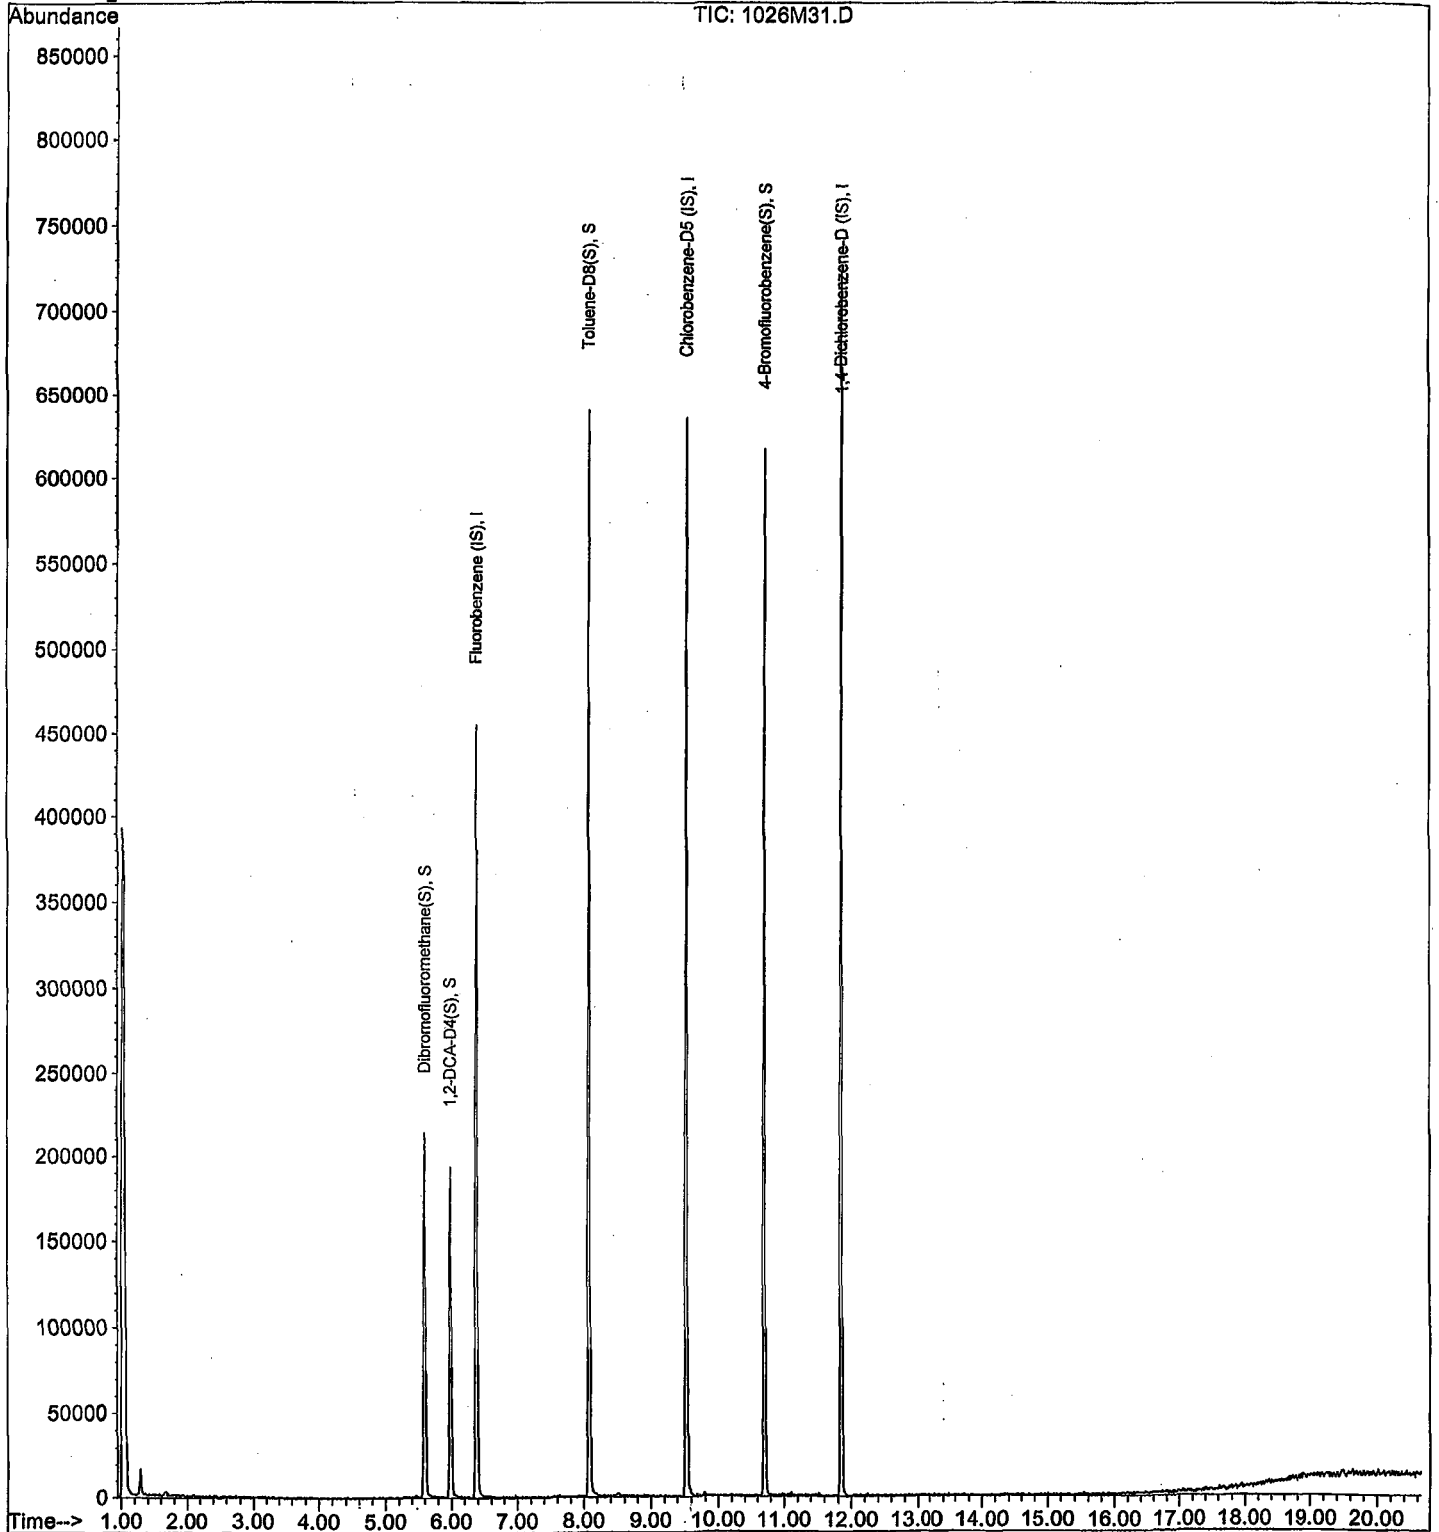

Data File : M:\MAX\DATA\211015\1026M26.D
 Acq On : 26 Oct 21 20:58
 Sample : 211026B LCS 10ug/L
 Misc : IS&S 8/4/21

Vial: 26
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 27 7:38 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 14:01:48 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.37	96	384412	25.00	ppb	0.03
65) Chlorobenzene-D5 (IS)	9.53	117	344538	25.00	ppb	0.03
80) 1,4-Dichlorobenzene-D (IS)	11.85	152	230340	25.00	ppb	0.03
System Monitoring Compounds						
41) Dibromofluoromethane(S)	5.59	111	122707	25.70	ppb	0.03
Spiked Amount	25.000		Recovery	=	102.808%	
46) 1,2-DCA-D4(S)	5.98	65	86592	26.00	ppb	0.03
Spiked Amount	25.000		Recovery	=	104.016%	
66) Toluene-D8(S)	8.08	98	402333	25.41	ppb	0.03
Spiked Amount	25.000		Recovery	=	101.628%	
74) 4-Bromofluorobenzene(S)	10.70	95	165389	25.86	ppb	0.03
Spiked Amount	25.000		Recovery	=	103.436%	
Target Compounds						Qvalue
3) Dichlorodifluoromethane	1.20	85	19984	8.68	ppb	99
4) Freon 114	1.30	85	13756	10.67	ppb	75
5) Chloromethane	1.34	50	13070	9.52	ppb	95
6) Vinyl chloride	1.43	62	15016	8.87	ppb	99
8) Bromomethane	1.69	94	13995	9.78	ppb	96
9) Chloroethane	1.79	64	10463	9.59	ppb	# 86
10) Dichlorofluoromethane	1.99	67	37572	10.11	ppb	90
11) Trichlorofluoromethane	2.02	101	43384	9.77	ppb	95
13) Acrolein	2.46	56	24816	115.33	ppb	94
14) Acetone	2.63	43	22327	44.55	ppb	98
15) Freon-113	2.55	151	18363	10.16	ppb	97
16) Acetonitrile	2.96	41	14482	121.59	ppb	# 95
18) 1,2-Dichlorotrifluoroethan	1.99	67	37572	10.11	ppb	100
19) 1,1-DCE	2.53	61	25598	9.51	ppb	98
20) t-Butanol	3.37	59	20369	131.21	ppb	97
21) Methyl Acetate	3.02	43	9041	10.73	ppb	# 83
22) Iodomethane	2.68	142	17296	9.33	ppb	94
23) Acrylonitrile	3.48	53	5326	11.24	ppb	# 73
25) Methylene chloride	3.12	84	18885	10.87	ppb	98
26) Carbon disulfide	2.74	76	20448	9.34	ppb	95
27) Methyl t-butyl ether (MtBE)	3.50	73	60960	10.52	ppb	# 89
28) Trans-1,2-DCE	3.46	96	18564	9.89	ppb	99
29) 3-Methylpentane	3.51	57	9651	9.83	ppb	86
31) Diisopropyl Ether	4.28	45	39861	11.03	ppb	98
32) 1,1-DCA	4.10	63	31658	11.25	ppb	# 96
34) Ethyl tert Butyl Ether	4.81	59	48057	10.35	ppb	96
35) Methylcyclopentane	4.81	56	2400	12.29	ppb	100

(#) = qualifier out of range (m) = manual integration

Data File : M:\MAX\DATA\211015\1026M26.D
 Acq On : 26 Oct 21 20:58
 Sample : 211026B LCS 10ug/L
 Misc : IS&S 8/4/21

Vial: 26
 Operator: LP, DG, CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 27 7:38 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 14:01:48 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
36) MEK (2-Butanone)	5.02	43	26982	51.49	ppb	86
37) Cis-1,2-DCE	4.95	96	21298	10.25	ppb	91
38) 2,2-Dichloropropane	4.93	77	34519	9.56	ppb	97
39) Chloroform	5.39	83	41439	11.34	ppb	90
40) Bromochloromethane	5.26	130	17390	10.72	ppb	# 86
42) 1,1,1-TCA	5.58	97	45090	10.51	ppb	96
43) Cyclohexane	5.62	41	12084	9.84	ppb	92
44) 1,1-Dichloropropene	5.79	75	24590	10.56	ppb	90
45) 2,2,4-Trimethylpentane	6.15	57	30250	10.02	ppb	# 81
47) Carbon Tetrachloride	5.77	117	41812	10.36	ppb	97
48) Tert Amyl Methyl Ether	6.22	73	48944	10.69	ppb	# 92
49) 1,2-DCA	6.07	62	37862	10.48	ppb	# 91
50) Benzene	6.03	78	69821	10.36	ppb	99
51) TCE	6.78	95	21827	10.11	ppb	87
52) 2-Pentanone	7.04	43	115184	131.50	ppb	94
53) 1,2-Dichloropropane	7.03	63	7230	9.65	ppb	99
54) Bromodichloromethane	7.34	83	32251	10.66	ppb	100
55) Methyl Cyclohexane	6.97	83	22916	9.88	ppb	95
56) Dibromomethane	7.15	93	12891	9.79	ppb	93
57) MIBK (methyl isobutyl ket	8.01	43	59671	53.27	ppb	96
58) 1-Bromo-2-chloroethane	7.65	144	4613	10.89	ppb	89
60) Cis-1,3-Dichloropropene	7.82	75	28050	10.35	ppb	91
61) Toluene	8.15	91	79977	10.26	ppb	96
62) Trans-1,3-Dichloropropene	8.40	75	30309	11.27	ppb	90
63) 1,1,2-TCA	8.57	83	13277	10.99	ppb	92
64) 2-Hexanone	8.85	43	39288	51.86	ppb	97
67) 1,2-EDB	9.06	107	18318	10.08	ppb	97
68) Tetrachloroethene	8.69	164	17976	10.00	ppb	83
69) 1-Chlorohexane	9.56	91	13192	9.65	ppb	94
70) 1,1,1,2-Tetrachloroethane	9.65	131	28007	10.93	ppb	96
71) m&p-Xylene	9.80	106	81214	20.85	ppb	92
72) o-Xylene	10.19	106	41665	10.20	ppb	100
73) Styrene	10.20	104	66482	10.81	ppb	98
75) 1,3-Dichloropropane	8.74	76	28707	10.74	ppb	94
76) Dibromochloromethane	8.96	129	27788	10.39	ppb	99
77) Chlorobenzene	9.56	112	61589	10.31	ppb	95
78) Ethylbenzene	9.68	91	97805	10.35	ppb	96
79) Bromoform	10.37	173	22727	10.24	ppb	99
81) Isopropylbenzene	10.56	105	108731	10.12	ppb	96
82) 1,1,2,2-Tetrachloroethane	10.87	83	18621	10.10	ppb	90
83) 1,2,3-Trichloropropane	10.90	110	8542	9.27	ppb	90
84) t-1,4-Dichloro-2-Butene	10.93	53	3999	8.57	ppb	98

(#) = qualifier out of range (m) = manual integration

Data File : M:\MAX\DATA\211015\1026M26.D
 Acq On : 26 Oct 21 20:58
 Sample : 211026B LCS 10ug/L
 Misc : IS&S 8/4/21

Vial: 26
 Operator: LP, DG, CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 27 7:38 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 14:01:48 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
85) Bromobenzene	10.84	156	37902	10.78	ppb	96
86) n-Propylbenzene	10.97	91	111766	10.54	ppb	98
87) 4-Ethyltoluene	11.08	105	102540	10.47	ppb	96
88) 2-Chlorotoluene	11.04	91	86101	10.24	ppb	92
89) 1,3,5-Trimethylbenzene	11.15	105	93508	10.20	ppb	97
90) 4-Chlorotoluene	11.15	91	88144	10.55	ppb	97
91) Tert-Butylbenzene	11.47	119	55664	11.00	ppb	98
92) 1,2,4-Trimethylbenzene	11.51	105	97292	11.20	ppb	99
93) Sec-Butylbenzene	11.68	105	104546	10.80	ppb	97
94) p-Isopropyltoluene	11.83	119	102704	10.97	ppb	99
95) Benzyl Chloride	12.01	91	20416	9.21	ppb #	88
96) 1,3-DCB	11.78	146	64107	10.47	ppb	97
97) 1,4-DCB	11.87	146	61606	9.88	ppb	92
98) n-Butylbenzene	12.24	91	62443	9.89	ppb	95
99) 1,2-DCB	12.24	146	62773	10.48	ppb	95
100) Hexachloroethane	12.48	117	17913	11.42	ppb	88
101) 1,2-Dibromo-3-chloropropan	13.02	75	4863	9.35	ppb	85
102) 1,2,4-Trichlorobenzene	13.84	180	20568	8.79	ppb	92
103) Hexachlorobutadiene	14.01	225	24853	9.72	ppb	96
104) Naphthalene	14.08	128	43249	9.86	ppb	99
105) 1,2,3-Trichlorobenzene	14.32	180	27435	9.03	ppb	93

(#) = qualifier out of range (m) = manual integration

Quantitation Report


Data File : M:\MAX\DATA\211015\1026M26.D
Acq On : 26 Oct 21 20:58
Sample : 211026B LCS 10ug/L
Misc : IS&S 8/4/21

Vial: 26
Operator: LP,DG, CH
Inst : Max
Multiplr: 1.00

Quant Time: Oct 27 7:38 2021

Quant Results File: M1015W.RES

Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
Title : METHOD 8260B
Last Update : Sat Oct 16 14:01:48 2021
Response via : Initial Calibration

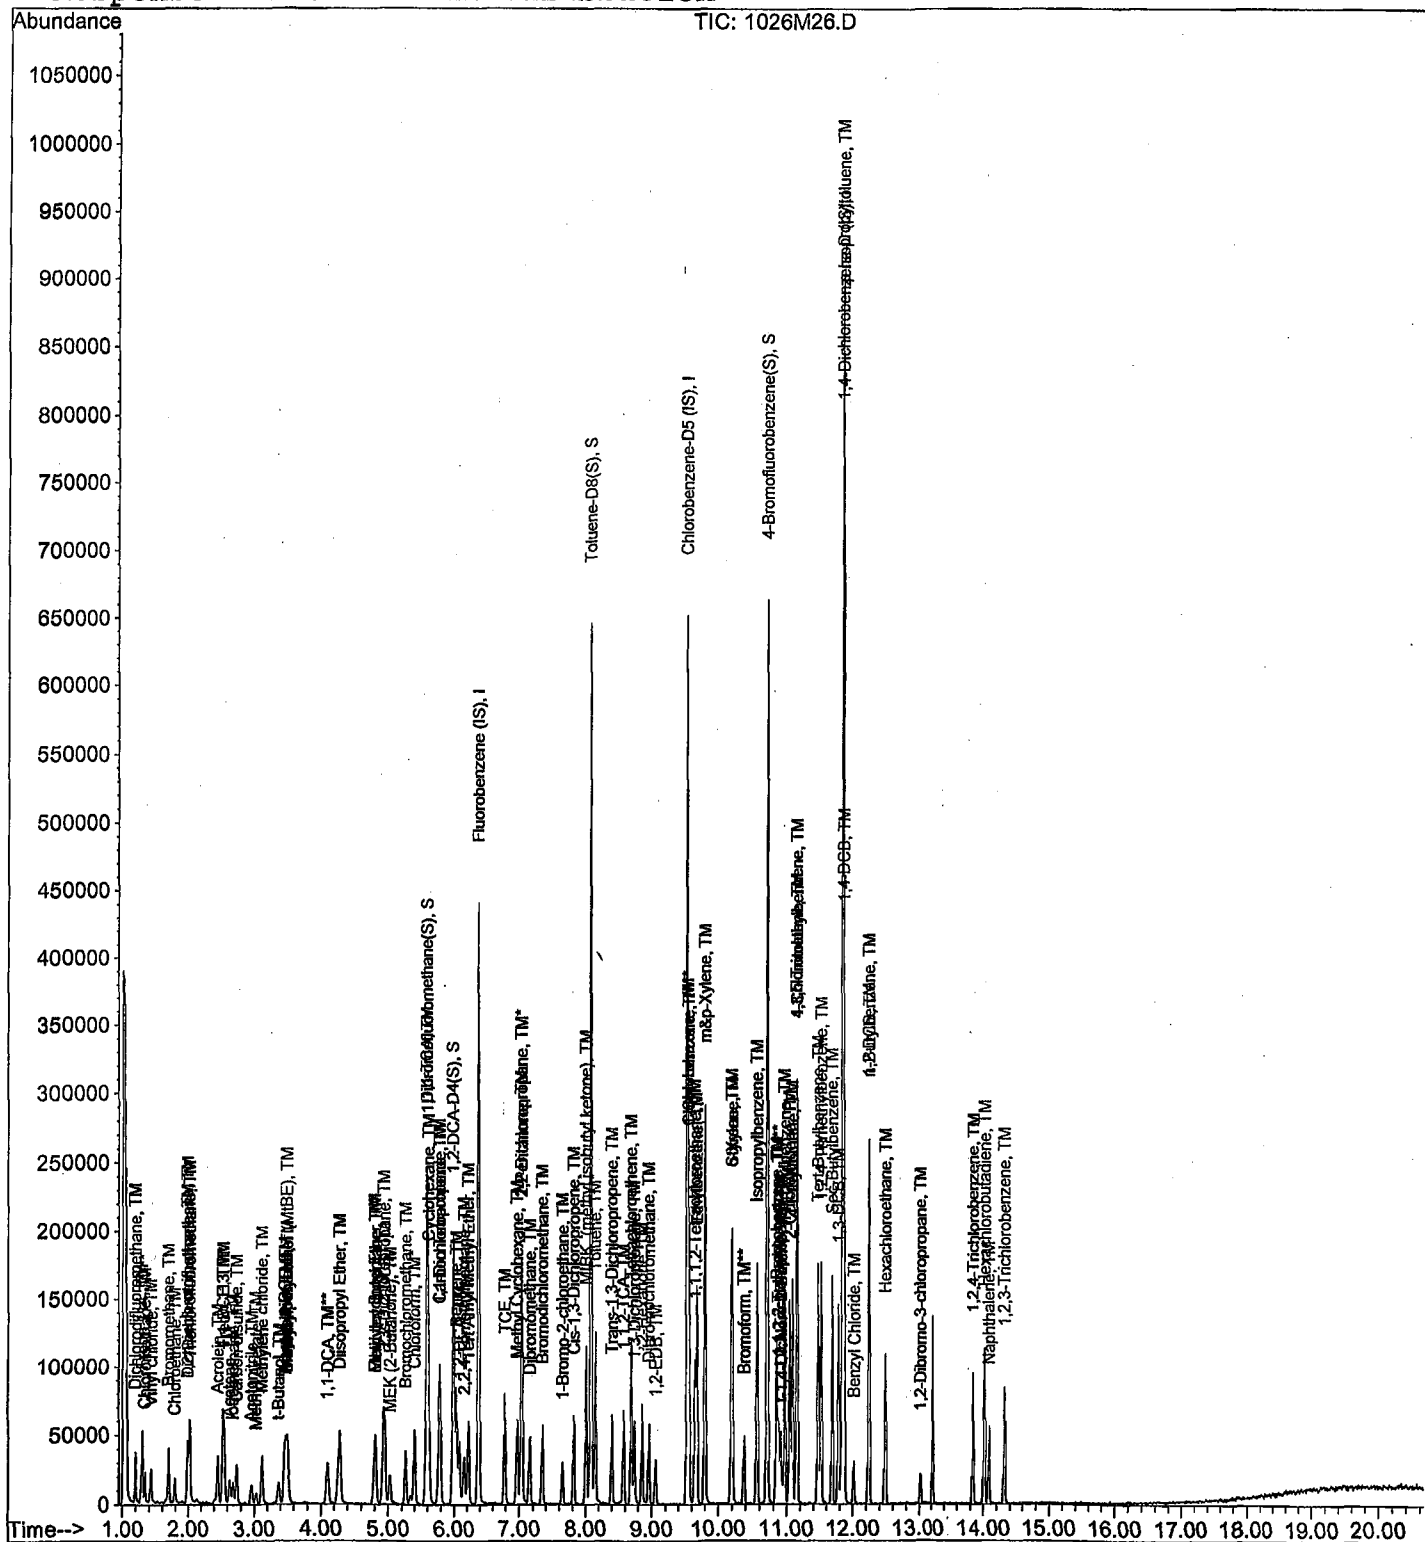

Data File : M:\MAX\DATA\211015\1026M27.D
 Acq On : 26 Oct 21 21:26
 Sample : 211026B LCSD 10ug/L
 Misc : IS&S 8/4/21

Vial: 27
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 27 7:38 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 14:01:48 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.37	96	379540	25.00	ppb	0.03
65) Chlorobenzene-D5 (IS)	9.53	117	341797	25.00	ppb	0.03
80) 1,4-Dichlorobenzene-D (IS)	11.85	152	227568	25.00	ppb	0.03

System Monitoring Compounds

41) Dibromofluoromethane (S)	5.59	111	121442	25.76	ppb	0.03
Spiked Amount	25.000		Recovery	=	103.052%	
46) 1,2-DCA-D4 (S)	5.98	65	82992	25.24	ppb	0.03
Spiked Amount	25.000		Recovery	=	100.972%	
66) Toluene-D8 (S)	8.08	98	395294	25.16	ppb	0.03
Spiked Amount	25.000		Recovery	=	100.648%	
74) 4-Bromofluorobenzene (S)	10.70	95	162229	25.57	ppb	0.03
Spiked Amount	25.000		Recovery	=	102.276%	

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Dichlorodifluoromethane	1.20	85	18448	8.12	ppb	99
4) Freon 114	1.30	85	12941	10.17	ppb	79
5) Chloromethane	1.34	50	11148	8.22	ppb	95
6) Vinyl chloride	1.43	62	13302	7.96	ppb	98
8) Bromomethane	1.69	94	13105	9.28	ppb	93
9) Chloroethane	1.79	64	8411	8.01	ppb	92
10) Dichlorofluoromethane	1.99	67	33622	9.17	ppb	99
11) Trichlorofluoromethane	2.02	101	37801	8.62	ppb	100
13) Acrolein	2.46	56	20810	98.24	ppb	97
14) Acetone	2.63	43	22743	45.96	ppb	97
15) Freon-113	2.55	151	17544	9.83	ppb	91
16) Acetonitrile	2.96	41	13729	116.74	ppb	# 94
18) 1,2-Dichlorotrifluoroethan	1.99	67	33622	9.17	ppb	100
19) 1,1-DCE	2.53	61	23564	8.87	ppb	95
20) t-Butanol	3.38	59	20603	134.80	ppb	99
21) Methyl Acetate	3.03	43	8412	10.11	ppb	87
22) Iodomethane	2.68	142	15317	8.50	ppb	94
23) Acrylonitrile	3.46	53	4463	9.53	ppb	94
25) Methylene chloride	3.12	84	16196	9.44	ppb	96
26) Carbon disulfide	2.74	76	19960	9.23	ppb	98
27) Methyl t-butyl ether (MtBE)	3.50	73	53922	9.42	ppb	100
28) Trans-1,2-DCE	3.46	96	17307	9.34	ppb	92
29) 3-Methylpentane	3.50	57	9164	9.43	ppb	97
31) Diisopropyl Ether	4.28	45	35859	10.05	ppb	# 84
32) 1,1-DCA	4.10	63	29327	10.55	ppb	# 93
34) Ethyl tert Butyl Ether	4.80	59	43521	9.49	ppb	99
35) Methylcyclopentane	4.81	56	1668	8.23	ppb	100

(#) = qualifier out of range (m) = manual integration

Data File : M:\MAX\DATA\211015\1026M27.D
 Acq On : 26 Oct 21 21:26
 Sample : 211026B LCSD 10ug/L
 Misc : IS&S 8/4/21

Vial: 27
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 27 7:38 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 14:01:48 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
36) MEK (2-Butanone)	5.03	43	25751	49.77	ppb	92
37) Cis-1,2-DCE	4.95	96	20052	9.77	ppb	94
38) 2,2-Dichloropropane	4.93	77	30984	8.69	ppb #	88
39) Chloroform	5.39	83	37375	10.36	ppb	97
40) Bromochloromethane	5.26	130	14997	9.30	ppb #	89
42) 1,1,1-TCA	5.57	97	42969	10.14	ppb	99
43) Cyclohexane	5.62	41	12080	9.97	ppb	89
44) 1,1-Dichloropropene	5.79	75	22879	9.95	ppb	91
45) 2,2,4-Trimethylpentane	6.15	57	29533	9.91	ppb #	81
47) Carbon Tetrachloride	5.77	117	38944	9.77	ppb	99
48) Tert Amyl Methyl Ether	6.22	73	44689	9.88	ppb	97
49) 1,2-DCA	6.07	62	33940	9.51	ppb	95
50) Benzene	6.03	78	61798	9.29	ppb	97
51) TCE	6.78	95	20559	9.65	ppb	85
52) 2-Pentanone	7.04	43	105643	122.16	ppb	97
53) 1,2-Dichloropropane	7.03	63	7469	10.11	ppb	98
54) Bromodichloromethane	7.34	83	29179	9.77	ppb	93
55) Methyl Cyclohexane	6.97	83	22401	9.78	ppb	91
56) Dibromomethane	7.15	93	11664	8.97	ppb	91
57) MIBK (methyl isobutyl ket	8.00	43	53500	48.37	ppb	96
58) 1-Bromo-2-chloroethane	7.65	144	3941	9.43	ppb	79
60) Cis-1,3-Dichloropropene	7.82	75	25368	9.48	ppb	95
61) Toluene	8.14	91	74142	9.63	ppb	98
62) Trans-1,3-Dichloropropene	8.40	75	26692	10.06	ppb	99
63) 1,1,2-TCA	8.58	83	11725	9.83	ppb	95
64) 2-Hexanone	8.86	43	36553	48.87	ppb #	88
67) 1,2-EDB	9.06	107	15633	8.67	ppb	81
68) Tetrachloroethene	8.69	164	16856	9.37	ppb #	78
69) 1-Chlorohexane	9.56	91	13529	9.97	ppb	92
70) 1,1,1,2-Tetrachloroethane	9.65	131	26092	10.26	ppb	97
71) m&p-Xylene	9.79	106	77153	19.97	ppb	95
72) o-Xylene	10.19	106	37951	9.37	ppb	100
73) Styrene	10.20	104	61424	10.07	ppb	96
75) 1,3-Dichloropropane	8.74	76	24861	9.38	ppb	93
76) Dibromochloromethane	8.96	129	24461	9.22	ppb	98
77) Chlorobenzene	9.55	112	58182	9.82	ppb	96
78) Ethylbenzene	9.68	91	92383	9.85	ppb	99
79) Bromoform	10.37	173	18412	8.36	ppb	95
81) Isopropylbenzene	10.56	105	102532	9.66	ppb	98
82) 1,1,2,2-Tetrachloroethane	10.87	83	13988	7.68	ppb	93
83) 1,2,3-Trichloropropane	10.90	110	8055	8.85	ppb	93
84) t-1,4-Dichloro-2-Butene	10.93	53	4590	9.91	ppb #	61

(#) = qualifier out of range (m) = manual integration

Data File : M:\MAX\DATA\211015\1026M27.D
 Acq On : 26 Oct 21 21:26
 Sample : 211026B LCSD 10ug/L
 Misc : IS&S 8/4/21

Vial: 27
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 27 7:38 2021

Quant Results File: M1015W.RES

Quant Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Sat Oct 16 14:01:48 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
85) Bromobenzene	10.84	156	33019	9.50	ppb	95
86) n-Propylbenzene	10.97	91	101016	9.64	ppb	97
87) 4-Ethyltoluene	11.08	105	97568	10.08	ppb	93
88) 2-Chlorotoluene	11.04	91	75814	9.12	ppb	86
89) 1,3,5-Trimethylbenzene	11.14	105	90851	10.03	ppb	95
90) 4-Chlorotoluene	11.15	91	80148	9.71	ppb	99
91) Tert-Butylbenzene	11.47	119	52984	10.60	ppb	98
92) 1,2,4-Trimethylbenzene	11.52	105	87443	10.19	ppb	98
93) Sec-Butylbenzene	11.68	105	99267	10.38	ppb	98
94) p-Isopropyltoluene	11.83	119	95492	10.33	ppb	97
95) Benzyl Chloride	12.01	91	16122	7.36	ppb	98
96) 1,3-DCB	11.78	146	57916	9.58	ppb	96
97) 1,4-DCB	11.87	146	55933	9.08	ppb	94
98) n-Butylbenzene	12.24	91	55660	9.05	ppb	93
99) 1,2-DCB	12.24	146	56825	9.60	ppb	99
100) Hexachloroethane	12.48	117	15029	9.70	ppb	98
101) 1,2-Dibromo-3-chloropropan	13.02	75	4647	9.08	ppb #	75
102) 1,2,4-Trichlorobenzene	13.84	180	20568	8.87	ppb	83
103) Hexachlorobutadiene	14.01	225	22661	9.05	ppb	98
104) Naphthalene	14.08	128	38540	9.02	ppb	97
105) 1,2,3-Trichlorobenzene	14.32	180	25370	8.62	ppb	85

(#) = qualifier out of range (m) = manual integration

Quantitation Report


Data File : M:\MAX\DATA\211015\1026M27.D
Acq On : 26 Oct 21 21:26
Sample : 211026B LCSD 10ug/L
Misc : IS&S 8/4/21

Vial: 27
Operator: LP,DG,CH
Inst : Max
Multiplr: 1.00

Quant Time: Oct 27 7:38 2021

Quant Results File: M1015W.RES

Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
Title : METHOD 8260B
Last Update : Sat Oct 16 14:01:48 2021
Response via : Initial Calibration


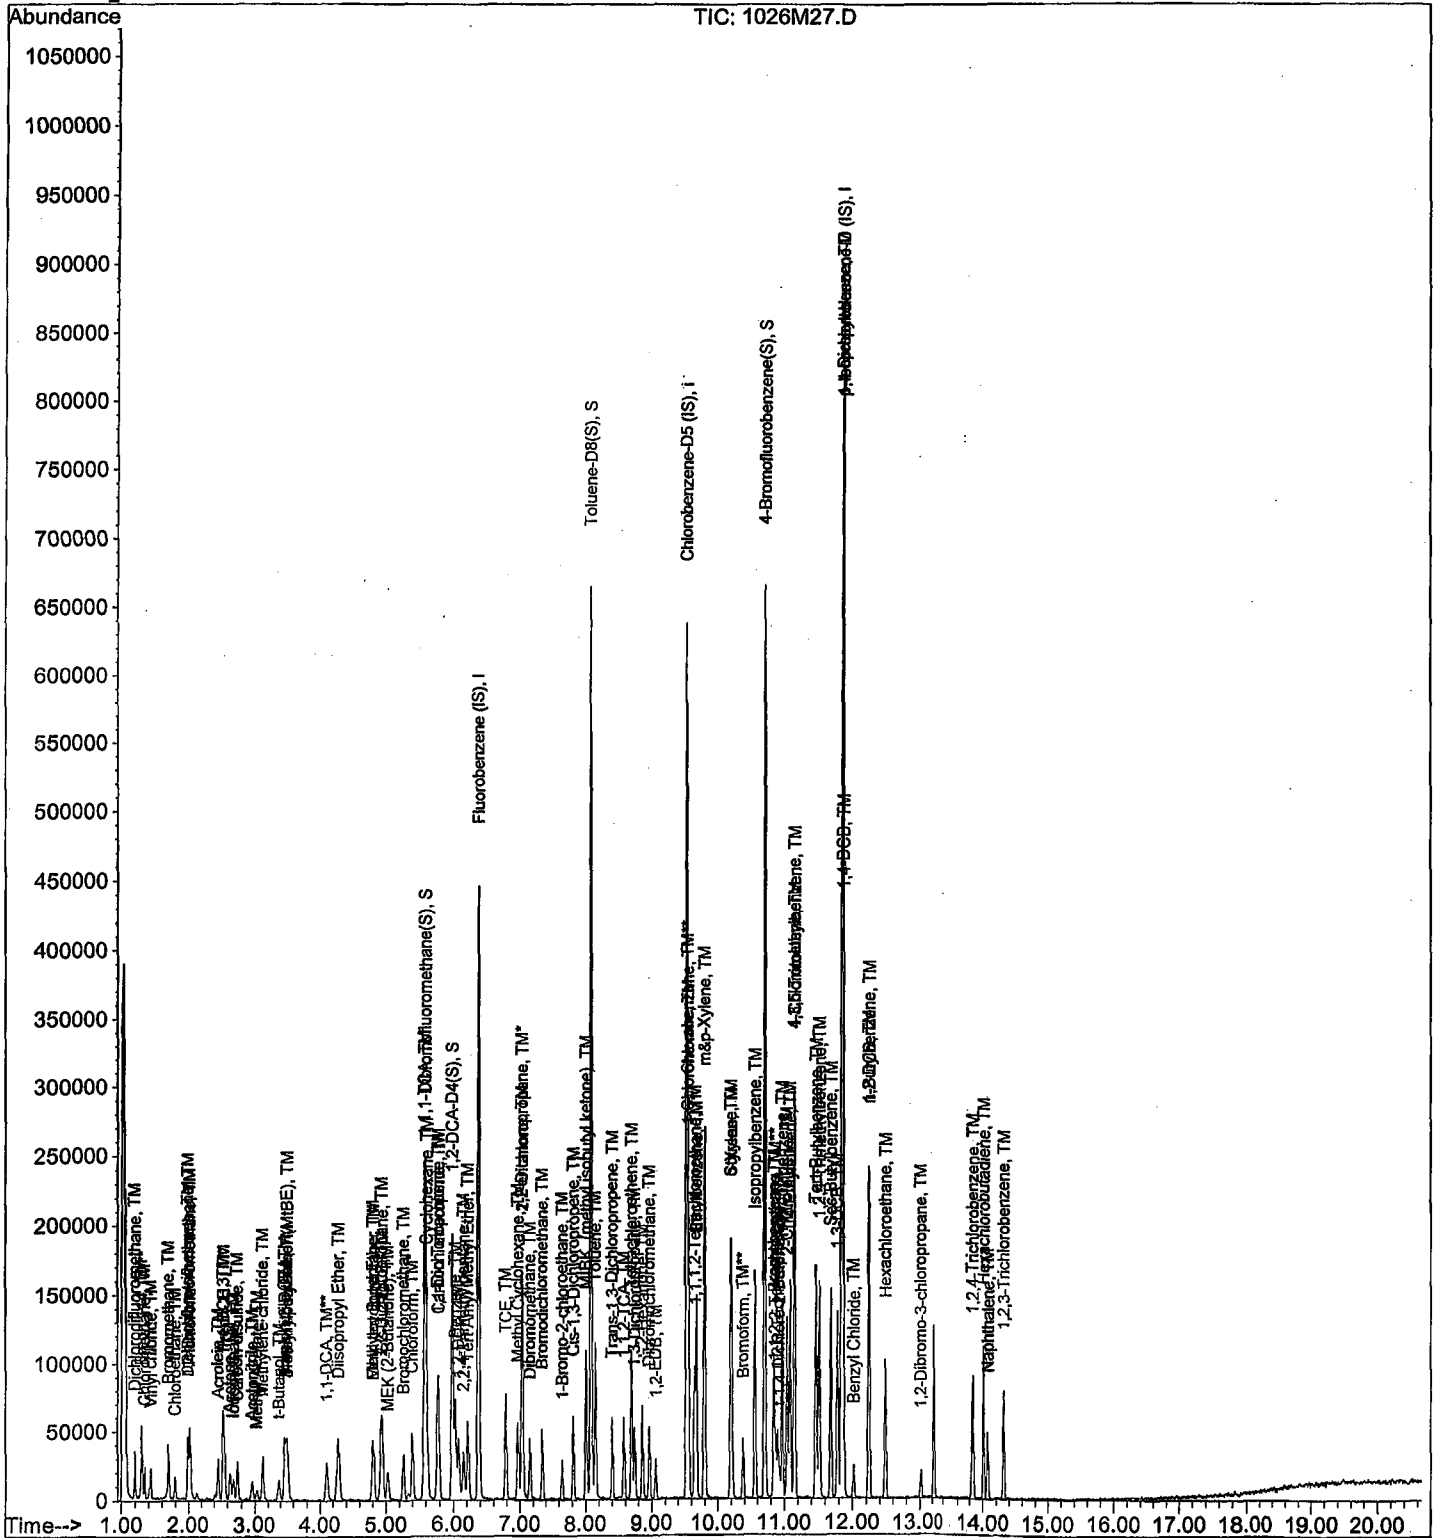


BFB

Data File : M:\MAX\DATA\211015\1015M11.D
 Acq On : 15 Oct 21 14:44
 Sample : 25ug/L BFB STD 9/23/21
 Misc : IS&S 8/4/21

Vial: 1
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B

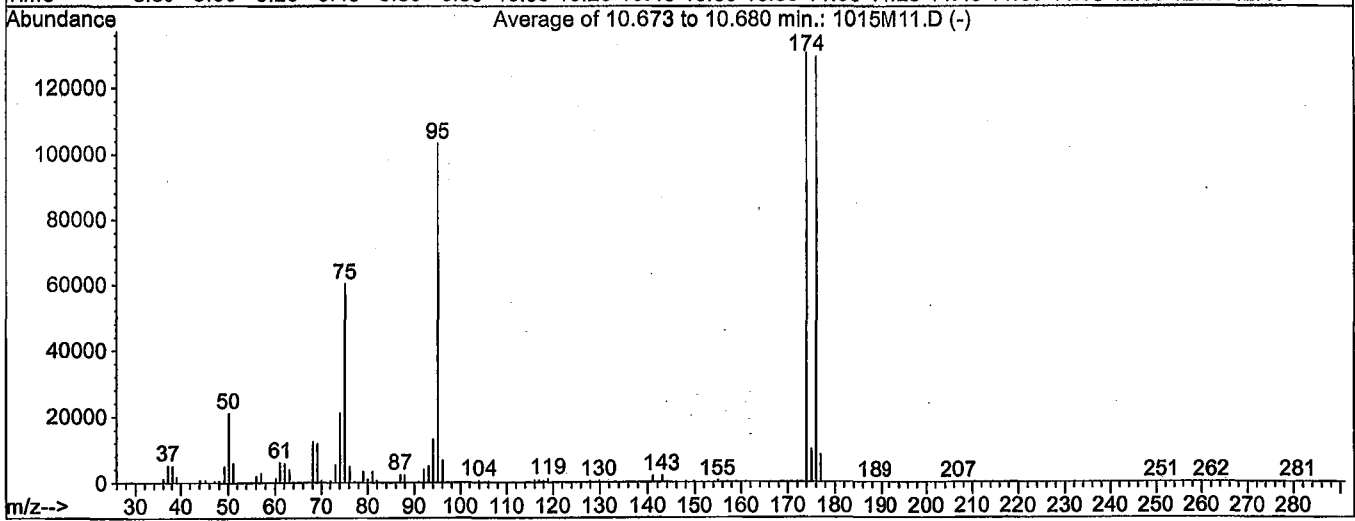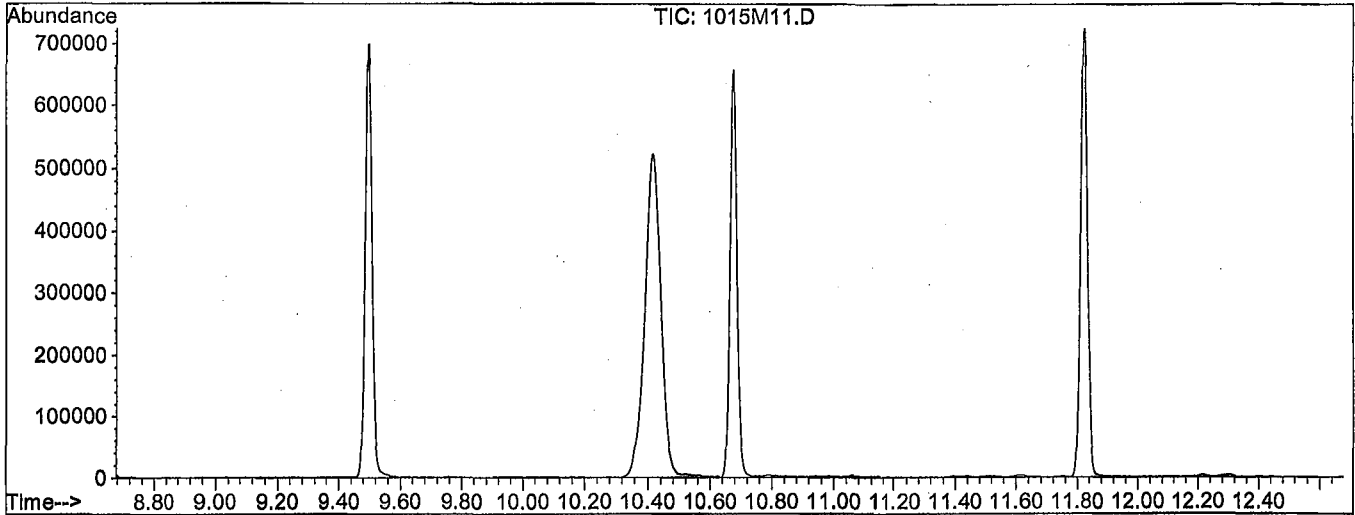

AutoFind: Scans 3033, 3034, 3035; Background Corrected with Scan 3020



Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	21096	PASS
75	95	30	60	58.4	60299	PASS
95	95	100	200	100.0	103195	PASS
96	95	5	9	6.7	6920	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	200	126.6	130632	PASS
175	174	5	9	7.7	10037	PASS
176	174	95	101	99.1	129467	PASS
177	176	5	9	6.5	8355	PASS

BFB

Data File : M:\MAX\DATA\211015\1026M24.D
 Acq On : 26 Oct 21 20:01
 Sample : 25ug/L BFB STD 9/23/21
 Misc : IS&S 8/4/21

Vial: 24
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Method : M:\MAX\DATA\211015\M1015W.M (RTE Integrator)
 Title : METHOD 8260B

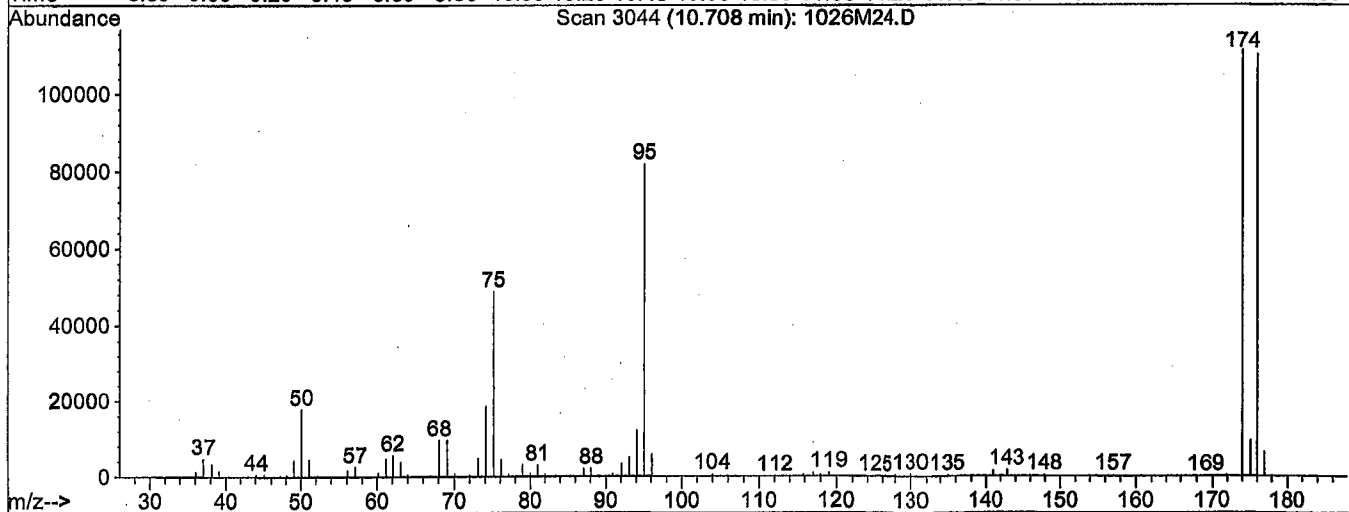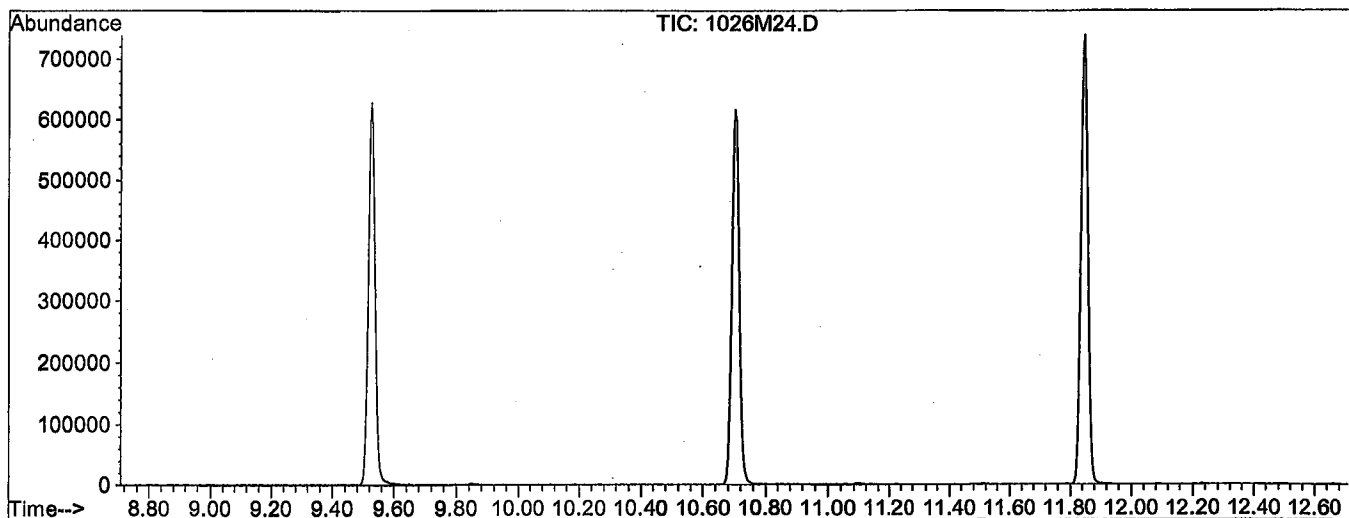

Spectrum Information: Scan 3044

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	17864	PASS
75	95	30	60	59.4	48664	PASS
95	95	100	200	100.0	81912	PASS
96	95	5	9	7.1	5855	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	200	136.3	111640	PASS
175	174	5	9	8.5	9455	PASS
176	174	95	101	98.9	110424	PASS
177	176	5	9	5.9	6466	PASS

MAX 8260 Standard Prep

MAX 8260 Water Calibration Curve										
0.3ug/L						Prepared By (Initials): CH				
Prepared: 8/25/2021										
Expires: 9/8/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 9	Various	0.3ug/L	5	Prepared 08/24/21	10/23/2021	N/A	3uL	50mL	P&T Water	0.3
VOA STD. 1	Absolute		50	Prepared 08/24/21	10/23/2021	N/A	5uL			5
VOA STD. 2	Phenova		100	Prepared 08/24/21	10/23/2021	N/A	2.5uL			5
VOA STD. TBA	Various		250	Prepared 08/24/21	9/8/2021	N/A	2uL			10
0.5ug/L										
Prepared: 8/25/2021										
Expires: 9/8/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 9	Various	0.5ug/L	5	Prepared 08/24/21	10/23/2021	N/A	5uL	50mL	P&T Water	0.5
VOA STD. 1	Absolute		50	Prepared 08/24/21	10/23/2021	N/A	10uL			10
VOA STD. 2	Phenova		100	Prepared 08/24/21	10/23/2021	N/A	5uL			10
VOA STD. TBA	Various		250	Prepared 08/24/21	9/8/2021	N/A	5uL			25
1.0ug/L										
Prepared: 8/25/2021										
Expires: 9/8/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 9	Various	1.0ug/L	5	Prepared 08/24/21	10/23/2021	N/A	10uL	50mL	P&T Water	1
VOA STD. 1	Absolute		50	Prepared 08/24/21	10/23/2021	N/A	20uL			20
VOA STD. 2	Phenova		100	Prepared 08/24/21	10/23/2021	N/A	10uL			20
VOA STD. TBA	Various		250	Prepared 08/24/21	9/8/2021	N/A	10uL			50
2.0ug/L										
Prepared: 8/25/2021										
Expires: 9/8/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 9	Various	2.0ug/L	5	Prepared 08/24/21	10/23/2021	N/A	20uL	50mL	P&T Water	2
VOA STD. 1	Absolute		50	Prepared 08/24/21	10/23/2021	N/A	30uL			30
VOA STD. 2	Phenova		100	Prepared 08/24/21	10/23/2021	N/A	15uL			30
VOA STD. TBA	Various		250	Prepared 08/24/21	9/8/2021	N/A	15uL			75
5ug/L										
Prepared: 8/25/2021										
Expires: 9/8/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	5ug/L	50	Prepared 08/24/21	10/23/2021	N/A	5uL	50mL	P&T Water	5
VOA STD. 8	Phenova		50	Prepared 08/24/21	9/8/2021	N/A	5uL			5
VOA STD. 1	Absolute		50	Prepared 08/24/21	10/23/2021	N/A	40uL			40
VOA STD. 2	Phenova		100	Prepared 08/24/21	10/23/2021	N/A	20uL			20
VOA STD. TBA	Various		250	Prepared 08/24/21	9/8/2021	N/A	20uL			100
10ug/L										
Prepared: 8/25/2021										
Expires: 9/8/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	10ug/L	50	Prepared 08/24/21	10/23/2021	N/A	10uL	50mL	P&T Water	10
VOA STD. 8	Phenova		50	Prepared 08/24/21	9/8/2021	N/A	10uL			10
VOA STD. 1	Absolute		50	Prepared 08/24/21	10/23/2021	N/A	50uL			50
VOA STD. 2	Phenova		100	Prepared 08/24/21	10/23/2021	N/A	25uL			50
VOA STD. TBA	Various		250	Prepared 08/24/21	9/8/2021	N/A	25uL			125

20ug/L										
Prepared: 8/25/2021										
Expires: 9/8/2021										
Initial Standard Information							Final Standard Information			
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	20ug/L	50	Prepared 08/24/21	10/23/2021	N/A	20uL	50mL	P&T Water	20
VOA STD. 8	Phenova		50	Prepared 08/24/21	10/23/2021	N/A	20uL			20
VOA STD. 1	Absolute		50	Prepared 08/24/21	10/23/2021	N/A	60uL			60
VOA STD. 2	Phenova		100	Prepared 08/24/21	10/23/2021	N/A	30uL			60
VOA STD. TBA	Various		250	Prepared 08/24/21	9/8/2021	N/A	30uL			150
40ug/L										
Prepared: 8/25/2021										
Expires: 9/8/2021										
Initial Standard Information							Final Standard Information			
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	40ug/L	50	Prepared 08/24/21	10/23/2021	N/A	40uL	50mL	P&T Water	40
VOA STD. 8	Phenova		50	Prepared 08/24/21	10/23/2021	N/A	40uL			40
VOA STD. 1	Absolute		50	Prepared 08/24/21	10/23/2021	N/A	80uL			80
VOA STD. 2	Phenova		100	Prepared 08/24/21	10/23/2021	N/A	40uL			80
VOA STD. TBA	Various		250	Prepared 08/24/21	9/8/2021	N/A	35uL			175
100ug/L										
Prepared: 8/25/2021										
Expires: 9/8/2021										
Initial Standard Information							Final Standard Information			
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	100ug/L	50	Prepared 08/24/21	10/23/2021	N/A	100uL	50mL	P&T Water	100
VOA STD. 8	Phenova		50	Prepared 08/24/21	10/23/2021	N/A	100uL			100
VOA STD. 1	Absolute		50	Prepared 08/24/21	10/23/2021	N/A	100uL			100
VOA STD. 2	Phenova		100	Prepared 08/24/21	10/23/2021	N/A	50uL			100
VOA STD. TBA	Various		250	Prepared 08/24/21	9/8/2021	N/A	40uL			200
MAX 8260 Water Second Source (SS)										
Prepared: 8/25/2021										
Expires: 9/8/2021										
Prepared By (Initials): CH										
Initial Standard Information							Final Standard Information			
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 3	Phenova	8260 Water SS	100	Prepared 08/24/21	10/23/2021	N/A	26uL	50mL	P&T Water	50
VOA STD. GASES	Phenova	8260 Water SS	50	Prepared 08/24/21	10/23/2021	N/A	10uL			10
VOA STD. 0	Phenova	8260 Water SS	50	Prepared 08/24/21	10/23/2021	N/A	10uL			10
VOA STD. 2-CEVE	Absolute	8260 Water SS	50	Prepared 08/24/21	8/24/2021	N/A	60uL			50
VOA STD. 6	Various	8260 Water SS	50	Prepared 08/24/21	9/8/2021	N/A	10uL			10
VOA STD. TBA	Various	8260 Water SS	250	Prepared 08/24/21	9/8/2021	N/A	25uL			250
8260 Water Continuing Calibrations (CCV)/ Lab Control Spikes (LCS)										
Prepared: 8/25/2021										
Expires: 8/26/2021										
Prepared By (Initials): CH										
Initial Standard Information							Final Standard Information			
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	CCV/ LCS	50	Prepared 08/24/21	10/23/2021	N/A	10uL	50mL	P&T Water	10
VOA STD. 8	Phenova	CCV/ LCS	50	Prepared 08/24/21	10/23/2021	N/A	10uL			10
VOA STD. 1	Absolute	CCV/ LCS	50	Prepared 08/24/21	10/23/2021	N/A	50uL			50
VOA STD. 2	Phenova	CCV/ LCS	100	Prepared 08/24/21	10/23/2021	N/A	25uL			50
VOA STD. TBA	Various	CCV/ LCS	250	Prepared 08/24/21	9/8/2021	N/A	25uL			250

MAX Gas Standard Prep

Gas Primary Working Standard										
Prepared: 6/23/2021						Prepared By (Initials): CH				
Expires: 1/4/2022										
Methanol Lot No.										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	Supplier P/N#	Conc. (ug/mL)	Lot Number - QA Number	Exp. Date (1 yr)	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/mL)
50,000ug/mL Gas STD	Restek	30205	50,000	A0132443	1/4/2022	12/31/2024	80uL	2mL	Methanol	2,000
Gas Second Source (SS) Working Standard										
Prepared: 3/31/2021						Prepared By (Initials): CH				
Expires: 1/31/1930										
Methanol Lot No.										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	Supplier P/N#	Conc. (ug/mL)	Lot Number - QA Number	Exp. Date (1 yr)	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/mL)
Gasoline (50,000ppm)	Phenova	ALO-101543	50,000	CL14915-51175	1/4/2022	1/31/1930	80uL	2mL	Methanol	2,000
MAX Gas Calibration Curve										
Prepared: 8/25/2021						Prepared By (Initials): CH				
Expires: 10/24/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA Gasses Standards	Phenova	20ug/L	2,000	Prepared 06/23/21	1/4/2022	N/A	1uL	100mL	P&T Water	20
VOA Gasses Standards	Phenova	50ug/L	2,000	Prepared 06/23/21	1/4/2022	N/A	2.5uL	100mL	P&T Water	50
VOA Gasses Standards	Phenova	100ug/L	2,000	Prepared 06/23/21	1/4/2022	N/A	5uL	100mL	P&T Water	100
VOA Gasses Standards	Phenova	300ug/L	2,000	Prepared 06/23/21	1/4/2022	N/A	15uL	100mL	P&T Water	300
VOA Gasses Standards	Phenova	600ug/L	2,000	Prepared 06/23/21	1/4/2022	N/A	30uL	100mL	P&T Water	600
VOA Gasses Standards	Phenova	800ug/L	2,000	Prepared 06/23/21	1/4/2022	N/A	40uL	100mL	P&T Water	800
VOA Gasses Standards	Phenova	1,000ug/L	2,000	Prepared 06/23/21	1/4/2022	N/A	50uL	100mL	P&T Water	1,000
Zeus Gas Second Source										
Prepared: 8/25/2021						Prepared By (Initials): CH				
Expires: 10/24/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
50,000ug/mL Gas STD	Phenova	SS 300ug/L	2,000	Prepared 03/31/21	1/31/1930	N/A	15uL	100mL	P&T Water	300
MAX Gas Continuing Calibrations/Lab Control Spikes										
Prepared: 8/25/2021						Prepared By (Initials): CH				
Expires: 8/26/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	Supplier P/N#	Conc. (ug/mL)	Lot Number - QA Number	Exp. Date (1 yr)	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/mL)
VOA Gasses Standards	Phenova	300ug/L	2,000	Prepared 06/23/21	1/4/2022	N/A	15uL	100mL	P&T Water	300

MAX 8260 Standard Prep

MAX 8260 Water Calibration Curve										
							Prepared By (Initials): <u>CH</u>			
0.3ug/L										
Prepared: 10/8/2021										
Expires: 10/20/2021										
Initial Standard Information							Final Standard Information			
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 9	Various	0.3ug/L	5	Prepared 10/07/21	12/6/2021	N/A	3uL	50mL	P&T Water	0.3
VOA STD. 1	Absolute		50	Prepared 10/07/21	12/6/2021	N/A	5uL			5
VOA STD. 2	Phenova		100	Prepared 10/07/21	12/6/2021	N/A	2.5uL			5
VOA STD. TBA	Various		250	Prepared 10/07/21	10/20/2021	N/A	2uL			10
0.5ug/L										
Prepared: 10/8/2021										
Expires: 10/20/2021										
Initial Standard Information							Final Standard Information			
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 9	Various	0.5ug/L	5	Prepared 10/07/21	12/6/2021	N/A	5uL	50mL	P&T Water	0.5
VOA STD. 1	Absolute		50	Prepared 10/07/21	12/6/2021	N/A	10uL			10
VOA STD. 2	Phenova		100	Prepared 10/07/21	12/6/2021	N/A	5uL			10
VOA STD. TBA	Various		250	Prepared 10/07/21	10/20/2021	N/A	5uL			25
1.0ug/L										
Prepared: 10/8/2021										
Expires: 10/20/2021										
Initial Standard Information							Final Standard Information			
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 9	Various	1.0ug/L	5	Prepared 10/07/21	12/6/2021	N/A	10uL	50mL	P&T Water	1
VOA STD. 1	Absolute		50	Prepared 10/07/21	12/6/2021	N/A	20uL			20
VOA STD. 2	Phenova		100	Prepared 10/07/21	12/6/2021	N/A	10uL			20
VOA STD. TBA	Various		250	Prepared 10/07/21	10/20/2021	N/A	10uL			50
2.0ug/L										
Prepared: 10/8/2021										
Expires: 10/20/2021										
Initial Standard Information							Final Standard Information			
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 9	Various	2.0ug/L	5	Prepared 10/07/21	12/6/2021	N/A	20uL	50mL	P&T Water	2
VOA STD. 1	Absolute		50	Prepared 10/07/21	12/6/2021	N/A	30uL			30
VOA STD. 2	Phenova		100	Prepared 10/07/21	12/6/2021	N/A	15uL			30
VOA STD. TBA	Various		250	Prepared 10/07/21	10/20/2021	N/A	15uL			75
5ug/L										
Prepared: 10/8/2021										
Expires: 10/20/2021										
Initial Standard Information							Final Standard Information			
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	5ug/L	50	Prepared 10/07/21	12/6/2021	N/A	5uL	50mL	P&T Water	5
VOA STD. 8	Phenova		50	Prepared 10/07/21	10/20/2021	N/A	5uL			5
VOA STD. 1	Absolute		50	Prepared 10/07/21	12/6/2021	N/A	40uL			40
VOA STD. 2	Phenova		100	Prepared 10/07/21	12/6/2021	N/A	20uL			20
VOA STD. TBA	Various		250	Prepared 10/07/21	10/20/2021	N/A	20uL			100
10ug/L										
Prepared: 10/8/2021										
Expires: 10/20/2021										
Initial Standard Information							Final Standard Information			
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	10ug/L	50	Prepared 10/07/21	12/6/2021	N/A	10uL	50mL	P&T Water	10
VOA STD. 8	Phenova		50	Prepared 10/07/21	10/20/2021	N/A	10uL			10
VOA STD. 1	Absolute		50	Prepared 10/07/21	12/6/2021	N/A	50uL			50
VOA STD. 2	Phenova		100	Prepared 10/07/21	12/6/2021	N/A	25uL			50
VOA STD. TBA	Various		250	Prepared 10/07/21	10/20/2021	N/A	25uL			125

20ug/L										
Prepared: 10/8/2021										
Expires: 10/20/2021										
Initial Standard Information							Final Standard Information			
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	20ug/L	50	Prepared 10/07/21	12/6/2021	N/A	20uL	50mL	P&T Water	20
VOA STD. 8	Phenova		50	Prepared 10/07/21	12/6/2021	N/A	20uL			20
VOA STD. 1	Absolute		50	Prepared 10/07/21	12/6/2021	N/A	60uL			60
VOA STD. 2	Phenova		100	Prepared 10/07/21	12/6/2021	N/A	30uL			60
VOA STD. TBA	Various		250	Prepared 10/07/21	12/6/2021	N/A	30uL			150
40ug/L										
Prepared: 10/8/2021										
Expires: 10/20/2021										
Initial Standard Information							Final Standard Information			
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	40ug/L	50	Prepared 10/07/21	12/6/2021	N/A	40uL	50mL	P&T Water	40
VOA STD. 8	Phenova		50	Prepared 10/07/21	12/6/2021	N/A	40uL			40
VOA STD. 1	Absolute		50	Prepared 10/07/21	12/6/2021	N/A	80uL			80
VOA STD. 2	Phenova		100	Prepared 10/07/21	12/6/2021	N/A	40uL			80
VOA STD. TBA	Various		250	Prepared 10/07/21	12/6/2021	N/A	35uL			175
100ug/L										
Prepared: 10/8/2021										
Expires: 10/20/2021										
Initial Standard Information							Final Standard Information			
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	100ug/L	50	Prepared 10/07/21	12/6/2021	N/A	100uL	50mL	P&T Water	100
VOA STD. 8	Phenova		50	Prepared 10/07/21	12/6/2021	N/A	100uL			100
VOA STD. 1	Absolute		50	Prepared 10/07/21	12/6/2021	N/A	100uL			100
VOA STD. 2	Phenova		100	Prepared 10/07/21	12/6/2021	N/A	50uL			100
VOA STD. TBA	Various		250	Prepared 10/07/21	12/6/2021	N/A	40uL			200
MAX 8260 Water Second Source (SS)										
Prepared: 10/8/2021										
Expires: 10/20/2021										
							Prepared By (Initials): CH			
Initial Standard Information							Final Standard Information			
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 3	Phenova	8260 Water SS	100	Prepared 10/07/21	12/6/2021	N/A	25uL	50mL	P&T Water	50
VOA STD. GASES	Phenova	8260 Water SS	50	Prepared 10/07/21	12/6/2021	N/A	10uL			10
VOA STD. 0	Phenova	8260 Water SS	50	Prepared 10/07/21	12/6/2021	N/A	10uL			10
VOA STD. 2-CEVE	Absolute	8260 Water SS	50	Prepared 10/07/21	10/7/2021	N/A	50uL			50
VOA STD. 6	Various	8260 Water SS	50	Prepared 10/07/21	10/20/2021	N/A	10uL			10
VOA STD. TBA	Various	8260 Water SS	250	Prepared 10/07/21	10/20/2021	N/A	25uL			250
8260 Water Continuing Calibrations (CCV/ Lab Control Spikes (LCS))										
Prepared: 10/8/2021										
Expires: 10/9/2021										
							Prepared By (Initials): CH			
Initial Standard Information							Final Standard Information			
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	CCV/ LCS	50	Prepared 10/07/21	12/6/2021	N/A	10uL	50mL	P&T Water	10
VOA STD. 8	Phenova	CCV/ LCS	50	Prepared 10/07/21	12/6/2021	N/A	10uL			10
VOA STD. 1	Absolute	CCV/ LCS	50	Prepared 10/07/21	12/6/2021	N/A	50uL			50
VOA STD. 2	Phenova	CCV/ LCS	100	Prepared 10/07/21	12/6/2021	N/A	25uL			50
VOA STD. TBA	Various	CCV/ LCS	250	Prepared 10/07/21	12/6/2021	N/A	25uL			250

Injection Log

Directory: M:\MAX\DATA\211015\

Line	Vial	FileName	Multiplier	SampleName	Misc Info	Injected
1	1	1015M11.D	1	25ug/L BFB STD 9/23/21	IS&S 8/4/21	15 Oct 21 14:44
2	2	1015M12.D	1	0.3ug/L VOC STD 10/15/21	IS&S 8/4/21	15 Oct 21 15:12
3	3	1015M13.D	1	0.5ug/L VOC STD 10/15/21	IS&S 8/4/21	15 Oct 21 15:41
4	4	1015M14.D	1	1ug/L VOC STD 10/15/21	IS&S 8/4/21	15 Oct 21 16:09
5	5	1015M15.D	1	2ug/L VOC STD 10/15/21	IS&S 8/4/21	15 Oct 21 16:38
6	6	1015M16.D	1	5ug/L VOC STD 10/15/21	IS&S 8/4/21	15 Oct 21 17:06
7	7	1015M17.D	1	10ug/L VOC STD 10/15/21	IS&S 8/4/21	15 Oct 21 17:35
8	8	1015M18.D	1	20ug/L VOC STD 10/15/21	IS&S 8/4/21	15 Oct 21 18:03
9	9	1015M19.D	1	40ug/L VOC STD 10/15/21	IS&S 8/4/21	15 Oct 21 18:31
10	10	1015M20.D	1	100ug/L VOC STD 10/15/21	IS&S 8/4/21	15 Oct 21 19:00
11	12	1015M22.D	1	(SS) 10ug/L VOC STD 10/15/21	IS&S 8/4/21	15 Oct 21 19:57

Injection Log

Directory: M:\MAX\DATA\211015\

Line	Vial	FileName	Multiplier	SampleName	Misc Info	Injected
1	24	1026M24.D	1	25ug/L BFB STD 9/23/21	IS&S 8/4/21	26 Oct 21 20:01
2	25	1026M25.D	1	211026B CCV 10ug/L	IS&S 8/4/21	26 Oct 21 20:30
3	26	1026M26.D	1	211026B LCS 10ug/L	IS&S 8/4/21	26 Oct 21 20:58
4	27	1026M27.D	1	211026B LCSD 10ug/L	IS&S 8/4/21	26 Oct 21 21:26
5	31	1026M31.D	1	211026B BLK	IS&S 8/4/21	26 Oct 21 23:20
6	35	1026M35.D	1	BA43836W01	IS&S 8/4/21	27 Oct 21 1:13
7	36	1026M36.D	1	BA43837W01	IS&S 8/4/21	27 Oct 21 1:41
8	45	1026M45.D	1	Ending CCV 10ug/L 10/26/21	IS&S 8/4/21	27 Oct 21 5:55

ORGANICS
Calibration Data

VOLATILE ORGANIC ANALYSIS BY
EPA METHOD 8260B

Form 6
Initial Calibration

Lab Name: APPL, Inc.
Case No: _____
Matrix: _____

SDG No: _____
Initial Cal. Date: 8/25/2021
Instrument: Max

Initials: _____

0825M12.D 0825M13.D 0825M14.D 0825M15.D 0825M16.D 0825M17.D 0825M18.D 0825M19.D 0825M20.D

	Compound	1	2	3	4	5	6	7	8	9		Avg	%RSD	Type	r^2	Q	MRF
1	I Fluorobenzene (IS)																
2	S Dibromofluoromethane(S)	0.3523	0.3417	0.2807	0.2859	0.2870	0.2956	0.2984	0.3009	0.2709		0.30	9.1	S			
3	S 1,2-DCA-D4(S)	0.2194	0.2154	0.1883	0.1930	0.1953	0.1908	0.1985	0.2034	0.1791		0.20	6.5	S			
4	I Chlorobenzene-D5 (IS)																
5	S Toluene-D8(S)	1.390	1.326	1.153	1.099	1.153	1.163	1.121	1.122	1.024		1.2	9.8	S			
6	S 4-Bromofluorobenzene(S)	0.5362	0.5171	0.4075	0.4294	0.4615	0.4643	0.4388	0.4514	0.4103		0.46	9.7	S			
7	I 1,4-Dichlorobenzene-D (IS)																
8																	
9																	
10																	
11																	
12																	
13																	
14																	
15																	
16																	
17																	
18																	
19																	
20																	
21																	
22																	
23																	
24																	
25																	
26																	
27																	
28																	
29																	
30																	
31																	
32																	
33																	
34																	
35																	

Data File : M:\MAX\DATA\210825\0825M12.D
 Acq On : 25 Aug 21 15:15
 Sample : 0.3ug/L VOC STD 8/25/21
 Misc : IS&S 6/4/21

Vial: 2
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Aug 26 15:25 2021

Quant Results File: M0825SUR.RES

Quant Method : M:\MAX\DATA\210825\M0825SUR.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Thu Aug 26 11:16:48 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260_081021

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.21	96	268418	25.00	ppb	0.00
4) Chlorobenzene-D5 (IS)	9.41	117	221472	25.00	ppb	0.00
7) 1,4-Dichlorobenzene-D (IS)	11.75	152	137587	25.00	ppb	0.00
System Monitoring Compounds						
2) Dibromofluoromethane(S)	5.41	111	18913	5.84	ppb	0.00
Spiked Amount	25.000		Recovery	=	23.372%	
3) 1,2-DCA-D4(S)	5.81	65	11779	5.54	ppb	0.00
Spiked Amount	25.000		Recovery	=	22.148%	
5) Toluene-D8(S)	7.95	98	61590	5.93	ppb	0.00
Spiked Amount	25.000		Recovery	=	23.720%	
6) 4-Bromofluorobenzene(S)	10.60	95	23749	5.86	ppb	0.00
Spiked Amount	25.000		Recovery	=	23.444%	

Target Compounds

Qvalue

Quantitation Report (Not Reviewed)

Data File : M:\MAX\DATA\210825\0825M13.D
 Acq On : 25 Aug 21 15:43
 Sample : 0.5ug/L VOC STD 8/25/21
 Misc : IS&S 6/4/21

Vial: 3
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Aug 26 15:25 2021

Quant Results File: M0825SUR.RES

Quant Method : M:\MAX\DATA\210825\M0825SUR.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Thu Aug 26 11:16:48 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260_081021

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.21	96	270425	25.00	ppb	0.00
4) Chlorobenzene-D5 (IS)	9.41	117	226950	25.00	ppb	0.00
7) 1,4-Dichlorobenzene-D (IS)	11.75	152	138629	25.00	ppb	0.00
System Monitoring Compounds						
2) Dibromofluoromethane(S)	5.42	111	18480	5.67	ppb	0.00
Spiked Amount	25.000		Recovery	=	22.664%	
3) 1,2-DCA-D4(S)	5.81	65	11650	5.44	ppb	0.00
Spiked Amount	25.000		Recovery	=	21.744%	
5) Toluene-D8(S)	7.95	98	60175	5.65	ppb	0.00
Spiked Amount	25.000		Recovery	=	22.616%	
6) 4-Bromofluorobenzene(S)	10.60	95	23472	5.65	ppb	0.00
Spiked Amount	25.000		Recovery	=	22.612%	
Target Compounds						Qvalue

Quantitation Report (Not Reviewed)

Data File : M:\MAX\DATA\210825\0825M14.D
 Acq On : 25 Aug 21 16:11
 Sample : 1ug/L VOC STD 8/25/21
 Misc : IS&S 6/4/21

Vial: 4
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Aug 26 15:25 2021

Quant Results File: M0825SUR.RES

Quant Method : M:\MAX\DATA\210825\M0825SUR.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Thu Aug 26 11:16:48 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260_081021

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.22	96	261019	25.00	ppb	0.00
4) Chlorobenzene-D5 (IS)	9.41	117	222702	25.00	ppb	0.00
7) 1,4-Dichlorobenzene-D (IS)	11.75	152	137225	25.00	ppb	0.00
System Monitoring Compounds						
2) Dibromofluoromethane(S)	5.41	111	29305	9.31	ppb	0.00
Spiked Amount	25.000		Recovery	=	37.236%	
3) 1,2-DCA-D4(S)	5.81	65	19664	9.51	ppb	0.00
Spiked Amount	25.000		Recovery	=	38.024%	
5) Toluene-D8(S)	7.95	98	102711	9.84	ppb	0.00
Spiked Amount	25.000		Recovery	=	39.340%	
6) 4-Bromofluorobenzene(S)	10.60	95	36297	8.91	ppb	0.00
Spiked Amount	25.000		Recovery	=	35.632%	
Target Compounds						Qvalue

Data File : M:\MAX\DATA\210825\0825M15.D
 Acq On : 25 Aug 21 16:39
 Sample : 2ug/L VOC STD 8/25/21
 Misc : IS&S 6/4/21

Vial: 5
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Aug 26 15:25 2021

Quant Results File: M0825SUR.RES

Quant Method : M:\MAX\DATA\210825\M0825SUR.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Thu Aug 26 11:16:48 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260_081021

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.21	96	260699	25.00	ppb	0.00
4) Chlorobenzene-D5 (IS)	9.42	117	218570	25.00	ppb	0.00
7) 1,4-Dichlorobenzene-D (IS)	11.75	152	137104	25.00	ppb	0.00
System Monitoring Compounds						
2) Dibromofluoromethane(S)	5.41	111	29818	9.48	ppb	0.00
Spiked Amount	25.000		Recovery	=	37.936%	
3) 1,2-DCA-D4(S)	5.82	65	20128	9.74	ppb	0.00
Spiked Amount	25.000		Recovery	=	38.968%	
5) Toluene-D8(S)	7.95	98	96059	9.37	ppb	0.00
Spiked Amount	25.000		Recovery	=	37.488%	
6) 4-Bromofluorobenzene(S)	10.60	95	37545	9.39	ppb	0.00
Spiked Amount	25.000		Recovery	=	37.556%	

Target Compounds

Qvalue

Data File : M:\MAX\DATA\210825\0825M16.D
 Acq On : 25 Aug 21 17:07
 Sample : 5ug/L VOC STD 8/25/21
 Misc : IS&S 6/4/21

Vial: 6
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Aug 26 15:25 2021

Quant Results File: M0825SUR.RES

Quant Method : M:\MAX\DATA\210825\M0825SUR.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Thu Aug 26 11:16:48 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260_081021

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.21	96	261599	25.00	ppb	0.00
4) Chlorobenzene-D5 (IS)	9.41	117	219379	25.00	ppb	0.00
7) 1,4-Dichlorobenzene-D (IS)	11.75	152	136215	25.00	ppb	0.00
System Monitoring Compounds						
2) Dibromofluoromethane(S)	5.41	111	75090	23.80	ppb	0.00
Spiked Amount	25.000		Recovery	=	95.204%	
3) 1,2-DCA-D4(S)	5.81	65	51096	24.65	ppb	0.00
Spiked Amount	25.000		Recovery	=	98.580%	
5) Toluene-D8(S)	7.95	98	252960	24.59	ppb	0.00
Spiked Amount	25.000		Recovery	=	98.356%	
6) 4-Bromofluorobenzene(S)	10.60	95	101253	25.23	ppb	0.00
Spiked Amount	25.000		Recovery	=	100.908%	

Target Compounds

Qvalue

Quantitation Report (Not Reviewed)

Data File : M:\MAX\DATA\210825\0825M17.D
 Acq On : 25 Aug 21 17:35
 Sample : 10ug/L VOC STD 8/25/21
 Misc : IS&S 6/4/21

Vial: 7
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Aug 26 15:25 2021

Quant Results File: M0825SUR.RES

Quant Method : M:\MAX\DATA\210825\M0825SUR.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Thu Aug 26 11:16:48 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260_081021

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.21	96	260876	25.00	ppb	0.00
4) Chlorobenzene-D5 (IS)	9.41	117	215380	25.00	ppb	0.00
7) 1,4-Dichlorobenzene-D (IS)	11.75	152	136295	25.00	ppb	0.00
System Monitoring Compounds						
2) Dibromofluoromethane(S)	5.42	111	77116	24.51	ppb	0.00
Spiked Amount	25.000		Recovery	=	98.044%	
3) 1,2-DCA-D4(S)	5.82	65	49768	24.07	ppb	0.00
Spiked Amount	25.000		Recovery	=	96.284%	
5) Toluene-D8(S)	7.95	98	250522	24.80	ppb	0.00
Spiked Amount	25.000		Recovery	=	99.216%	
6) 4-Bromofluorobenzene(S)	10.60	95	100010	25.38	ppb	0.00
Spiked Amount	25.000		Recovery	=	101.520%	

Target Compounds

Qvalue

Quantitation Report (Not Reviewed)

Data File : M:\MAX\DATA\210825\0825M18.D
 Acq On : 25 Aug 21 18:03
 Sample : 20ug/L VOC STD 8/25/21
 Misc : IS&S 6/4/21

Vial: 8
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Aug 26 15:25 2021

Quant Results File: M0825SUR.RES

Quant Method : M:\MAX\DATA\210825\M0825SUR.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Thu Aug 26 11:16:48 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260_081021

Internal Standards	R.T.	QI on	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.21	96	258006	25.00	ppb	0.00
4) Chlorobenzene-D5 (IS)	9.41	117	222674	25.00	ppb	0.00
7) 1,4-Dichlorobenzene-D (IS)	11.75	152	141752	25.00	ppb	0.00
System Monitoring Compounds						
2) Dibromofluoromethane (S)	5.42	111	153975	49.49	ppb	0.00
Spiked Amount	25.000					
					Recovery =	197.940%
3) 1,2-DCA-D4 (S)	5.81	65	102408	50.08	ppb	0.00
Spiked Amount	25.000					
					Recovery =	200.332%
5) Toluene-D8 (S)	7.95	98	499120	47.80	ppb	0.00
Spiked Amount	25.000					
					Recovery =	191.196%
6) 4-Bromofluorobenzene (S)	10.60	95	195414	47.97	ppb	0.00
Spiked Amount	25.000					
					Recovery =	191.868%
Target Compounds						Qvalue

Quantitation Report (Not Reviewed)

Data File : M:\MAX\DATA\210825\0825M19.D
 Acq On : 25 Aug 21 18:31
 Sample : 40ug/L VOC STD 8/25/21
 Misc : IS&S 6/4/21

Vial: 9
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Aug 26 15:25 2021

Quant Results File: M0825SUR.RES

Quant Method : M:\MAX\DATA\210825\M0825SUR.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Thu Aug 26 11:16:48 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260_081021

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.21	96	251853	25.00	ppb	0.00
4) Chlorobenzene-D5 (IS)	9.41	117	216925	25.00	ppb	0.00
7) 1,4-Dichlorobenzene-D (IS)	11.75	152	140689	25.00	ppb	0.00
System Monitoring Compounds						
2) Dibromofluoromethane(S)	5.41	111	151584	49.91	ppb	0.00
Spiked Amount	25.000		Recovery	=	199.628%	
3) 1,2-DCA-D4(S)	5.81	65	102456	51.33	ppb	0.00
Spiked Amount	25.000		Recovery	=	205.320%	
5) Toluene-D8(S)	7.95	98	486936	47.87	ppb	0.00
Spiked Amount	25.000		Recovery	=	191.472%	
6) 4-Bromofluorobenzene(S)	10.60	95	195822	49.34	ppb	0.00
Spiked Amount	25.000		Recovery	=	197.364%	

Target Compounds

Qvalue

Quantitation Report (Not Reviewed)

Data File : M:\MAX\DATA\210825\0825M20.D
 Acq On : 25 Aug 21 18:59
 Sample : 100ug/L VOC STD 8/25/21
 Misc : IS&S 6/4/21

Vial: 10
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Aug 26 15:25 2021

Quant Results File: M0825SUR.RES

Quant Method : M:\MAX\DATA\210825\M0825SUR.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Thu Aug 26 11:16:48 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260_081021

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.21	96	251268	25.00	ppb	0.00
4) Chlorobenzene-D5 (IS)	9.41	117	218191	25.00	ppb	0.00
7) 1,4-Dichlorobenzene-D (IS)	11.75	152	142788	25.00	ppb	0.00
System Monitoring Compounds						
2) Dibromofluoromethane(S)	5.42	111	272268	89.85	ppb	0.00
Spiked Amount	25.000		Recovery	=	359.396%	
3) 1,2-DCA-D4(S)	5.81	65	179968	90.37	ppb	0.00
Spiked Amount	25.000		Recovery	=	361.496%	
5) Toluene-D8(S)	7.95	98	893556	87.33	ppb	0.00
Spiked Amount	25.000		Recovery	=	349.324%	
6) 4-Bromofluorobenzene(S)	10.60	95	358053	89.70	ppb	0.00
Spiked Amount	25.000		Recovery	=	358.780%	

Target Compounds

Qvalue

VOLATILE ORGANIC ANALYSIS
VOLATILE ORGANIC COMPOUNDS

Form 6
Initial Calibration

Lab Name: APPL, Inc.
Case No: _____
Matrix: _____

SDG No: _____
Initial Cal. Date: 8/25/2021
Instrument: Max

Initials: _____

0825M23.D 0825M24.D 0825M25.D 0825M26.D 0825M27.D 0825M28.D 0825M29.D

	Compound	1	2	3	4	5	6	7				Avg	%RSD	Type	r ²	Q	MRF
1	I Fluorobenzene (IS)																
2	TMHB Gasoline C6-C10	13.8	5.689	3.019	1.290	0.8206	0.7117	0.6349				3.7	130	TMHB	0.999		
3	TMHB Chlorobenzene-D5 (IS)																
4	TMHB 1,4-Dichlorobenzene (IS)																
5																	
6																	
7																	
8																	
9																	
10																	
11																	
12																	
13																	
14																	
15																	
16																	
17																	
18																	
19																	
20																	
21																	
22																	
23																	
24																	
25																	
26																	
27																	
28																	
29																	
30																	
31																	
32																	
33																	
34																	
35																	

Quantitation Report (Not Reviewed)

Data File : M:\MAX\DATA\210825\0825M23.D
 Acq On : 25 Aug 21 20:23
 Sample : 20ug/L GAS STD 8/25/21
 Misc : IS&S 6/4/21

Vial: 13
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 29 14:41 2021

Quant Results File: MGAS0825.RES

Quant Method : M:\MAX\DATA\210825\MGAS0825.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Thu Aug 26 16:19:36 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260_081021

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.21	TIC	284811	25.00	ppb	0.00
3) Chlorobenzene-D5 (IS)	11.75	TIC	236410m	25.00	ppb	0.00
4) 1,4-Dichlorobenzene (IS)	10.94	TIC	14670m	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Gasoline C6-C10	7.95	TIC	2520945m	-126.62	ppb	100

Quantitation Report


Data File : M:\MAX\DATA\210825\0825M23.D
Acq On : 25 Aug 21 20:23
Sample : 20ug/L GAS STD 8/25/21
Misc : IS&S 6/4/21

Vial: 13
Operator: LP,DG,CH
Inst : Max
Multiplr: 1.00

Quant Time: Oct 29 14:41 2021

Quant Results File: MGAS0825.RES

Method : M:\MAX\DATA\211015\MGAS0825.M (RTE Integrator)
Title : METHOD 8260B
Last Update : Thu Aug 26 16:19:36 2021
Response via : Initial Calibration

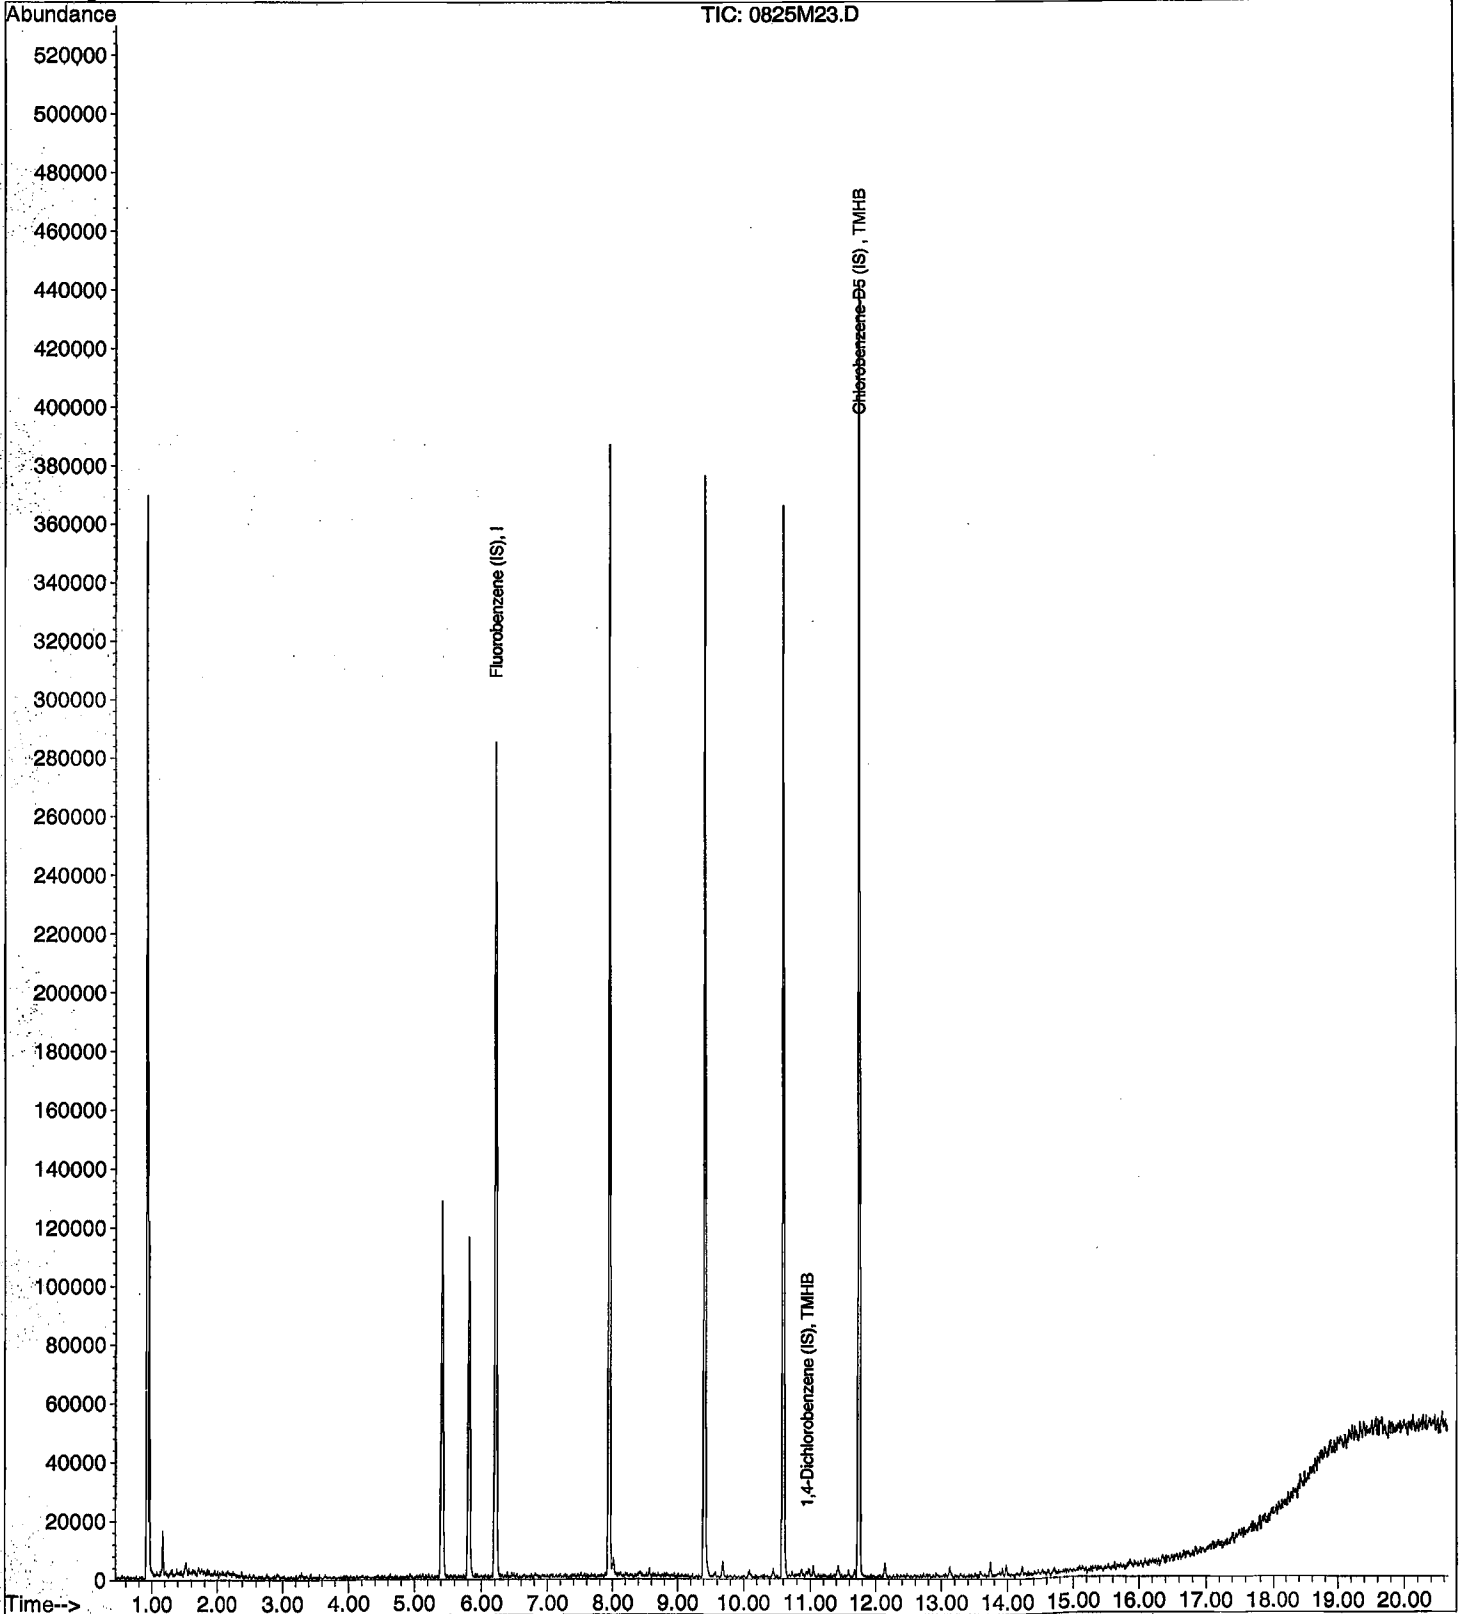

Quantitation Report (Not Reviewed)

Data File : M:\MAX\DATA\210825\0825M24.D
 Acq On : 25 Aug 21 20:51
 Sample : 50ug/L GAS STD 8/25/21
 Misc : IS&S 6/4/21

Vial: 14
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 29 14:41 2021

Quant Results File: MGAS0825.RES

Quant Method : M:\MAX\DATA\210825\MGAS0825.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Thu Aug 26 16:19:36 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260_081021

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.21	TIC	285081	25.00	ppb	0.00
3) Chlorobenzene-D5 (IS)	11.75	TIC	248593m	25.00	ppb	0.00
4) 1,4-Dichlorobenzene (IS)	10.94	TIC	21251m	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Gasoline C6-C10	7.95	TIC	2656639m	-95.17	ppb	100

Quantitation Report


Data File : M:\MAX\DATA\210825\0825M24.D
Acq On : 25 Aug 21 20:51
Sample : 50ug/L GAS STD 8/25/21
Misc : IS&S 6/4/21

Vial: 14
Operator: LP,DG,CH
Inst : Max
Multiplr: 1.00

Quant Time: Oct 29 14:41 2021

Quant Results File: MGAS0825.RES

Method : M:\MAX\DATA\211015\MGAS0825.M (RTE Integrator)
Title : METHOD 8260B
Last Update : Thu Aug 26 16:19:36 2021
Response via : Initial Calibration

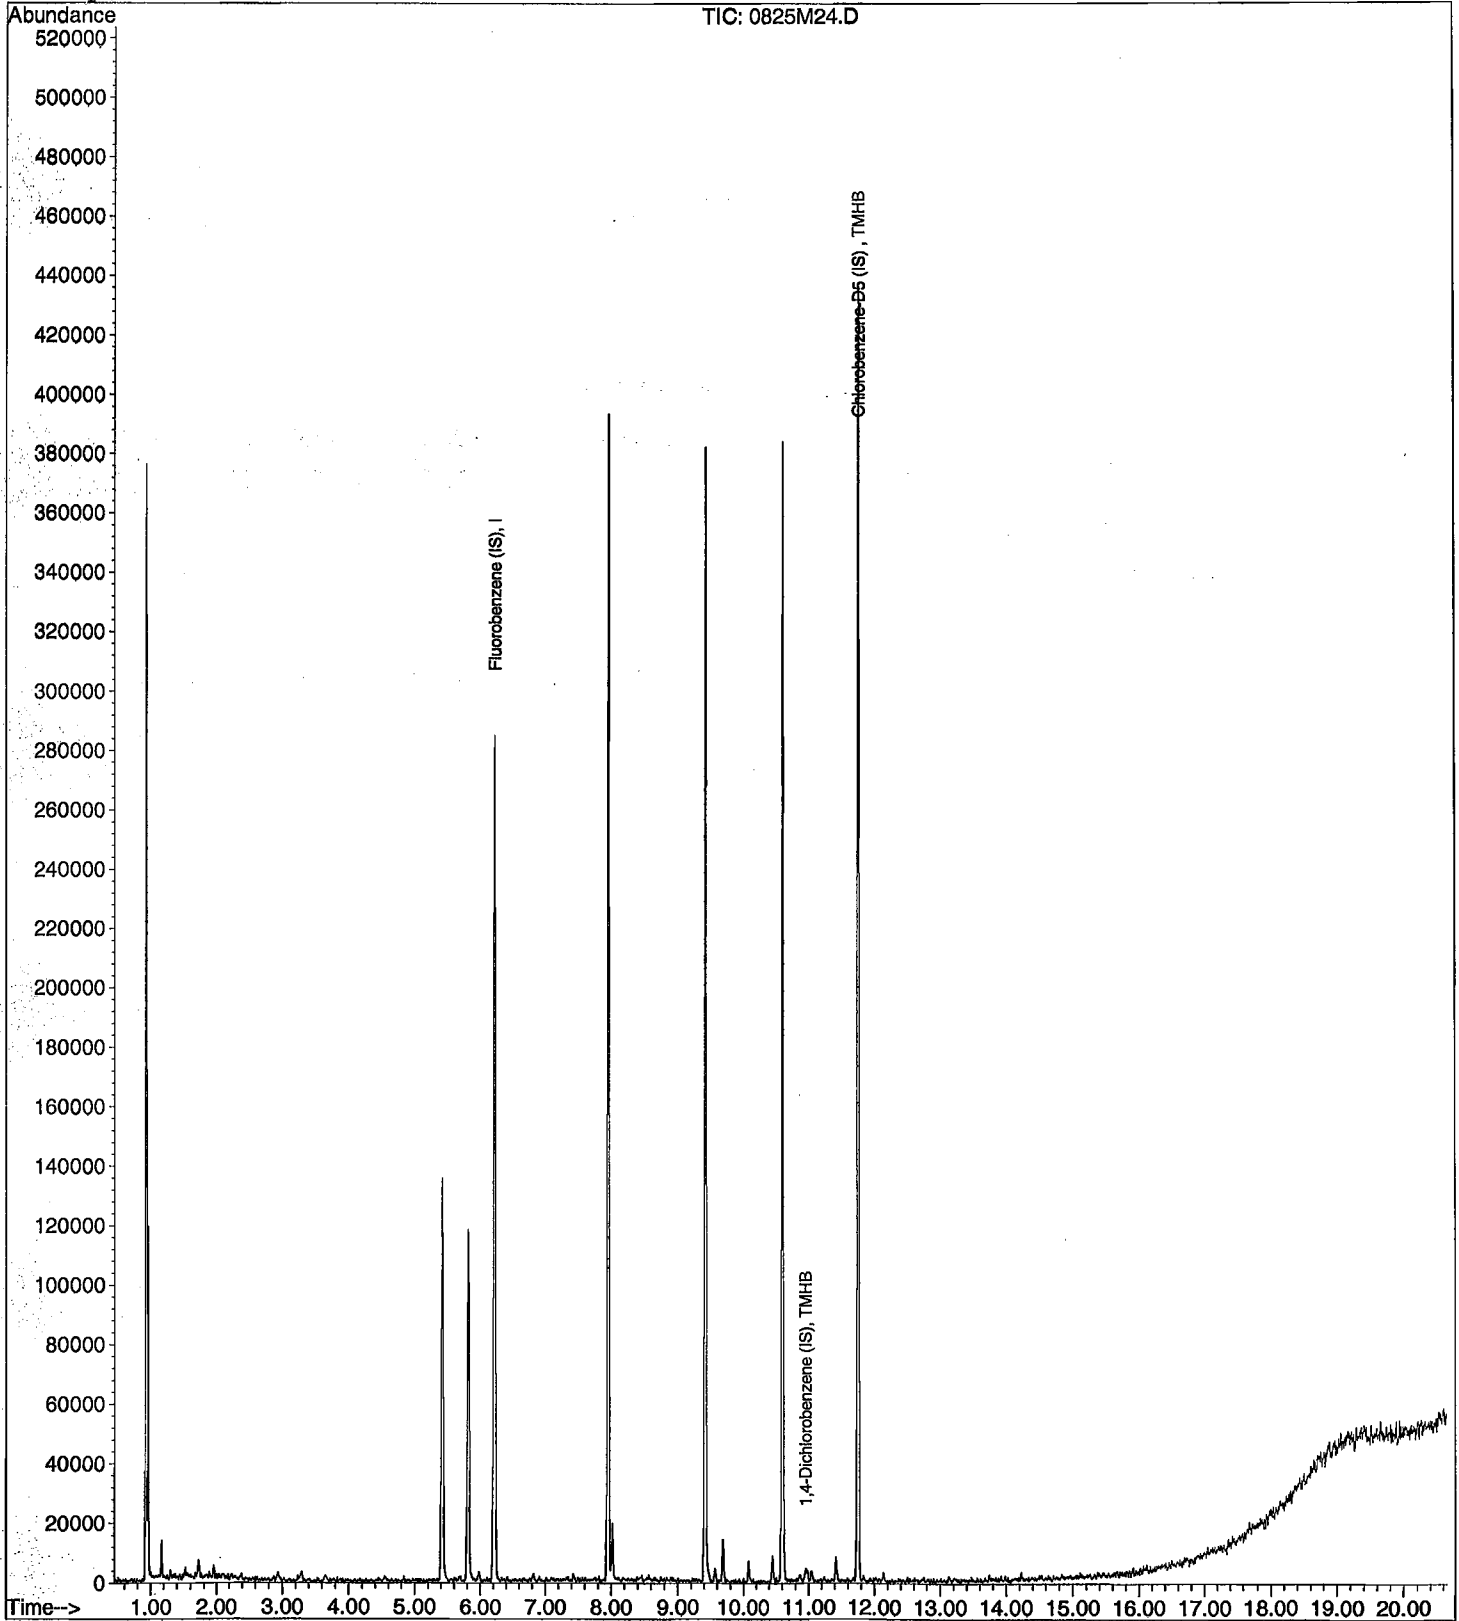

Quantitation Report (Not Reviewed)

Data File : M:\MAX\DATA\210825\0825M25.D
 Acq On : 25 Aug 21 21:19
 Sample : 100ug/L GAS STD 8/25/21
 Misc : IS&S 6/4/21

Vial: 15
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 29 14:41 2021

Quant Results File: MGAS0825.RES

Quant Method : M:\MAX\DATA\210825\MGAS0825.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Thu Aug 26 16:19:36 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260_081021

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.21	TIC	286586	25.00	ppb	0.00
3) Chlorobenzene-D5 (IS)	11.75	TIC	245880m	25.00	ppb	0.00
4) 1,4-Dichlorobenzene (IS)	10.94	TIC	32801m	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Gasoline C6-C10	7.95	TIC	2860551m	-50.60	ppb	100

Quantitation Report


Data File : M:\MAX\DATA\210825\0825M25.D
Acq On : 25 Aug 21 21:19
Sample : 100ug/L GAS STD 8/25/21
Misc : IS&S 6/4/21

Vial: 15
Operator: LP,DG,CH
Inst : Max
Multiplr: 1.00

Quant Time: Oct 29 14:41 2021

Quant Results File: MGAS0825.RES

Method : M:\MAX\DATA\211015\MGAS0825.M (RTE Integrator)
Title : METHOD 8260B
Last Update : Thu Aug 26 16:19:36 2021
Response via : Initial Calibration

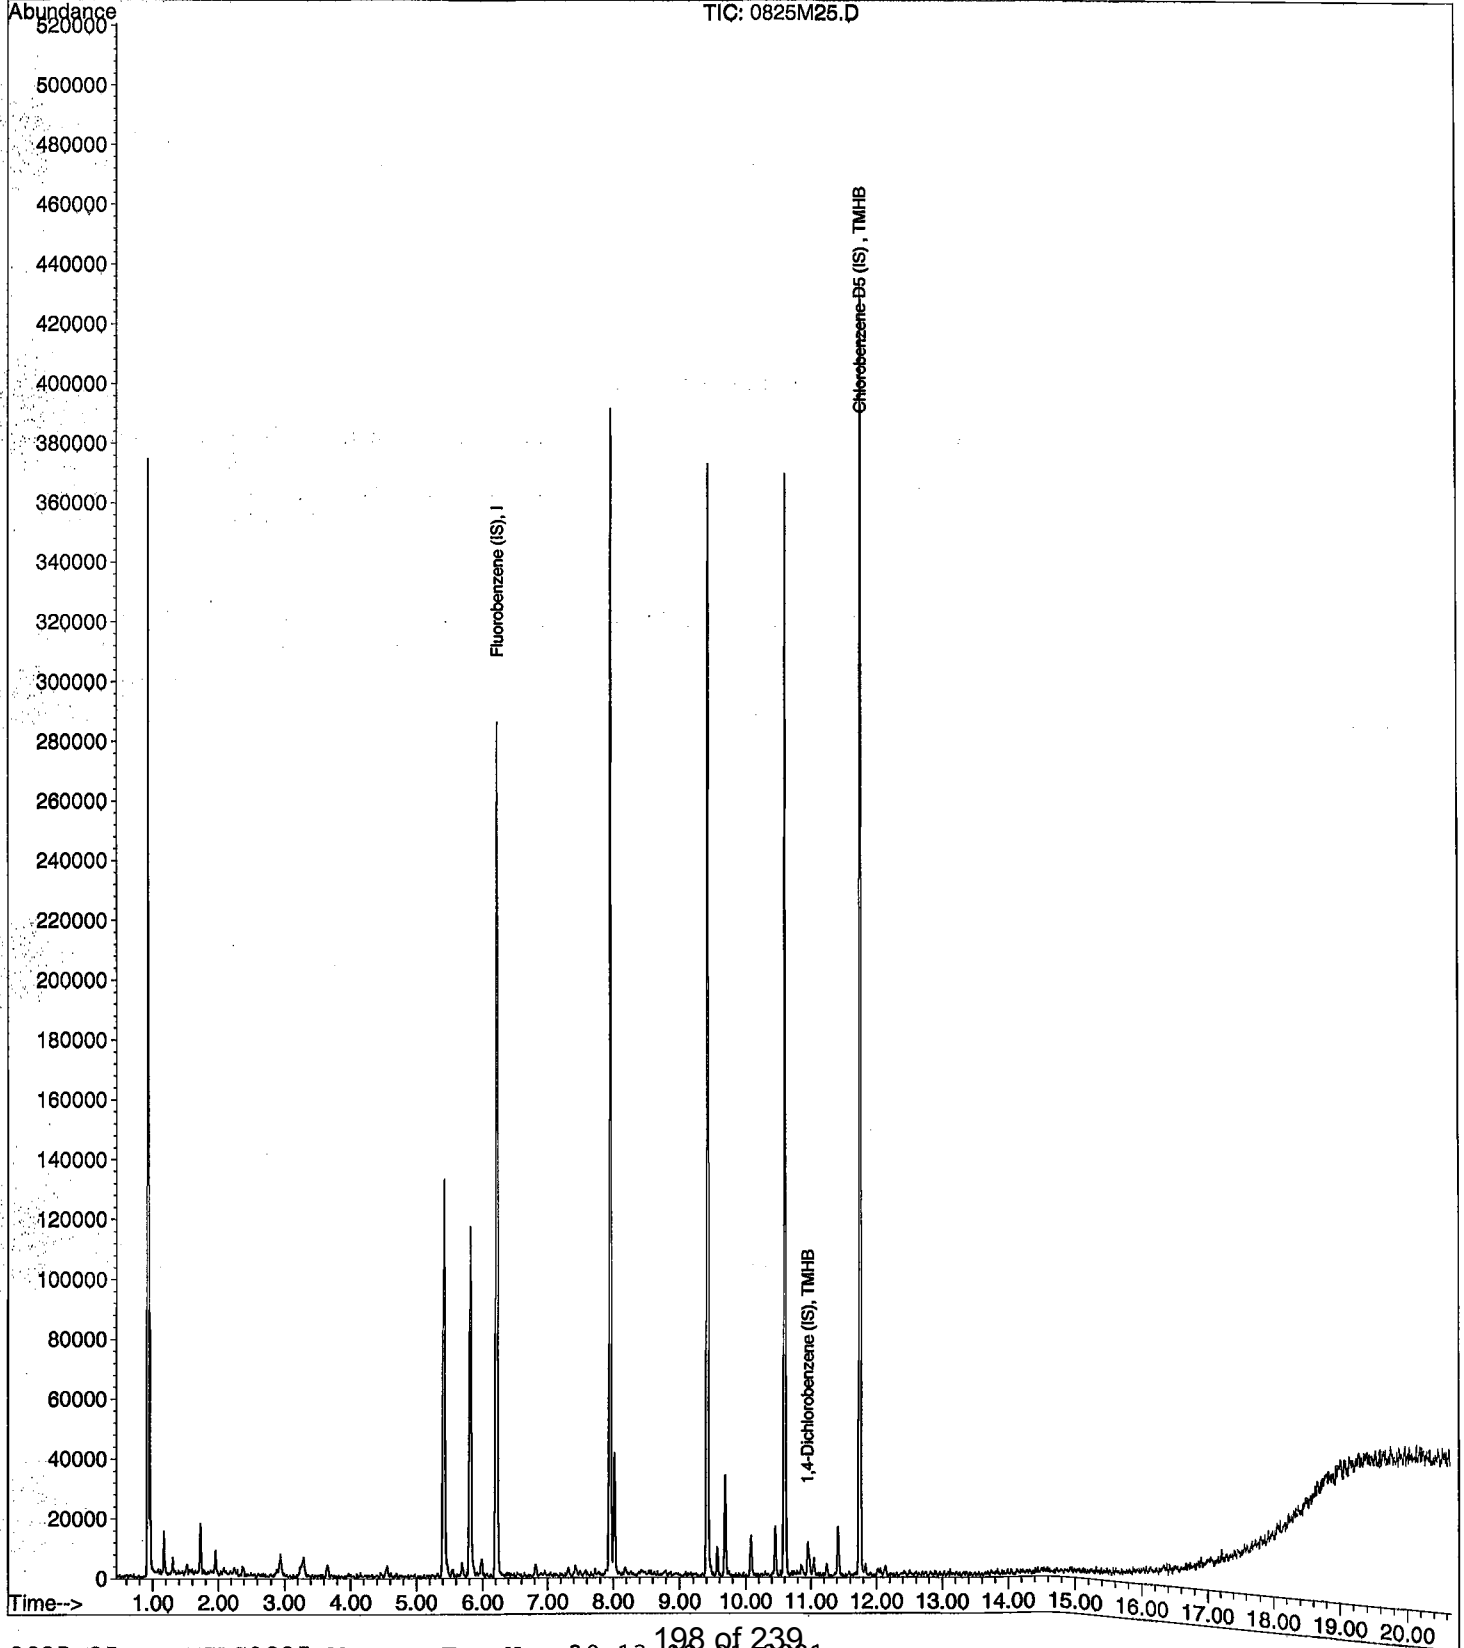

Quantitation Report (Not Reviewed)

Data File : M:\MAX\DATA\210825\0825M26.D
 Acq On : 25 Aug 21 21:47
 Sample : 300ug/L GAS STD 8/25/21
 Misc : IS&S 6/4/21

Vial: 16
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 29 14:41 2021

Quant Results File: MGAS0825.RES

Quant Method : M:\MAX\DATA\210825\MGAS0825.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Thu Aug 26 16:19:36 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260_081021

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.21	TIC	280163	25.00	ppb	0.00
3) Chlorobenzene-D5 (IS)	11.75	TIC	264646m	25.00	ppb	0.00
4) 1,4-Dichlorobenzene (IS)	10.94	TIC	87973m	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Gasoline C6-C10	7.95	TIC	3665952m	158.15	ppb	100

Quantitation Report


Data File : M:\MAX\DATA\210825\0825M26.D
Acq On : 25 Aug 21 21:47
Sample : 300ug/L GAS STD 8/25/21
Misc : IS&S 6/4/21

Vial: 16
Operator: LP,DG,CH
Inst : Max
Multiplr: 1.00

Quant Time: Oct 29 14:41 2021

Quant Results File: MGAS0825.RES

Method : M:\MAX\DATA\211015\MGAS0825.M (RTE Integrator)
Title : METHOD 8260B
Last Update : Thu Aug 26 16:19:36 2021
Response via : Initial Calibration

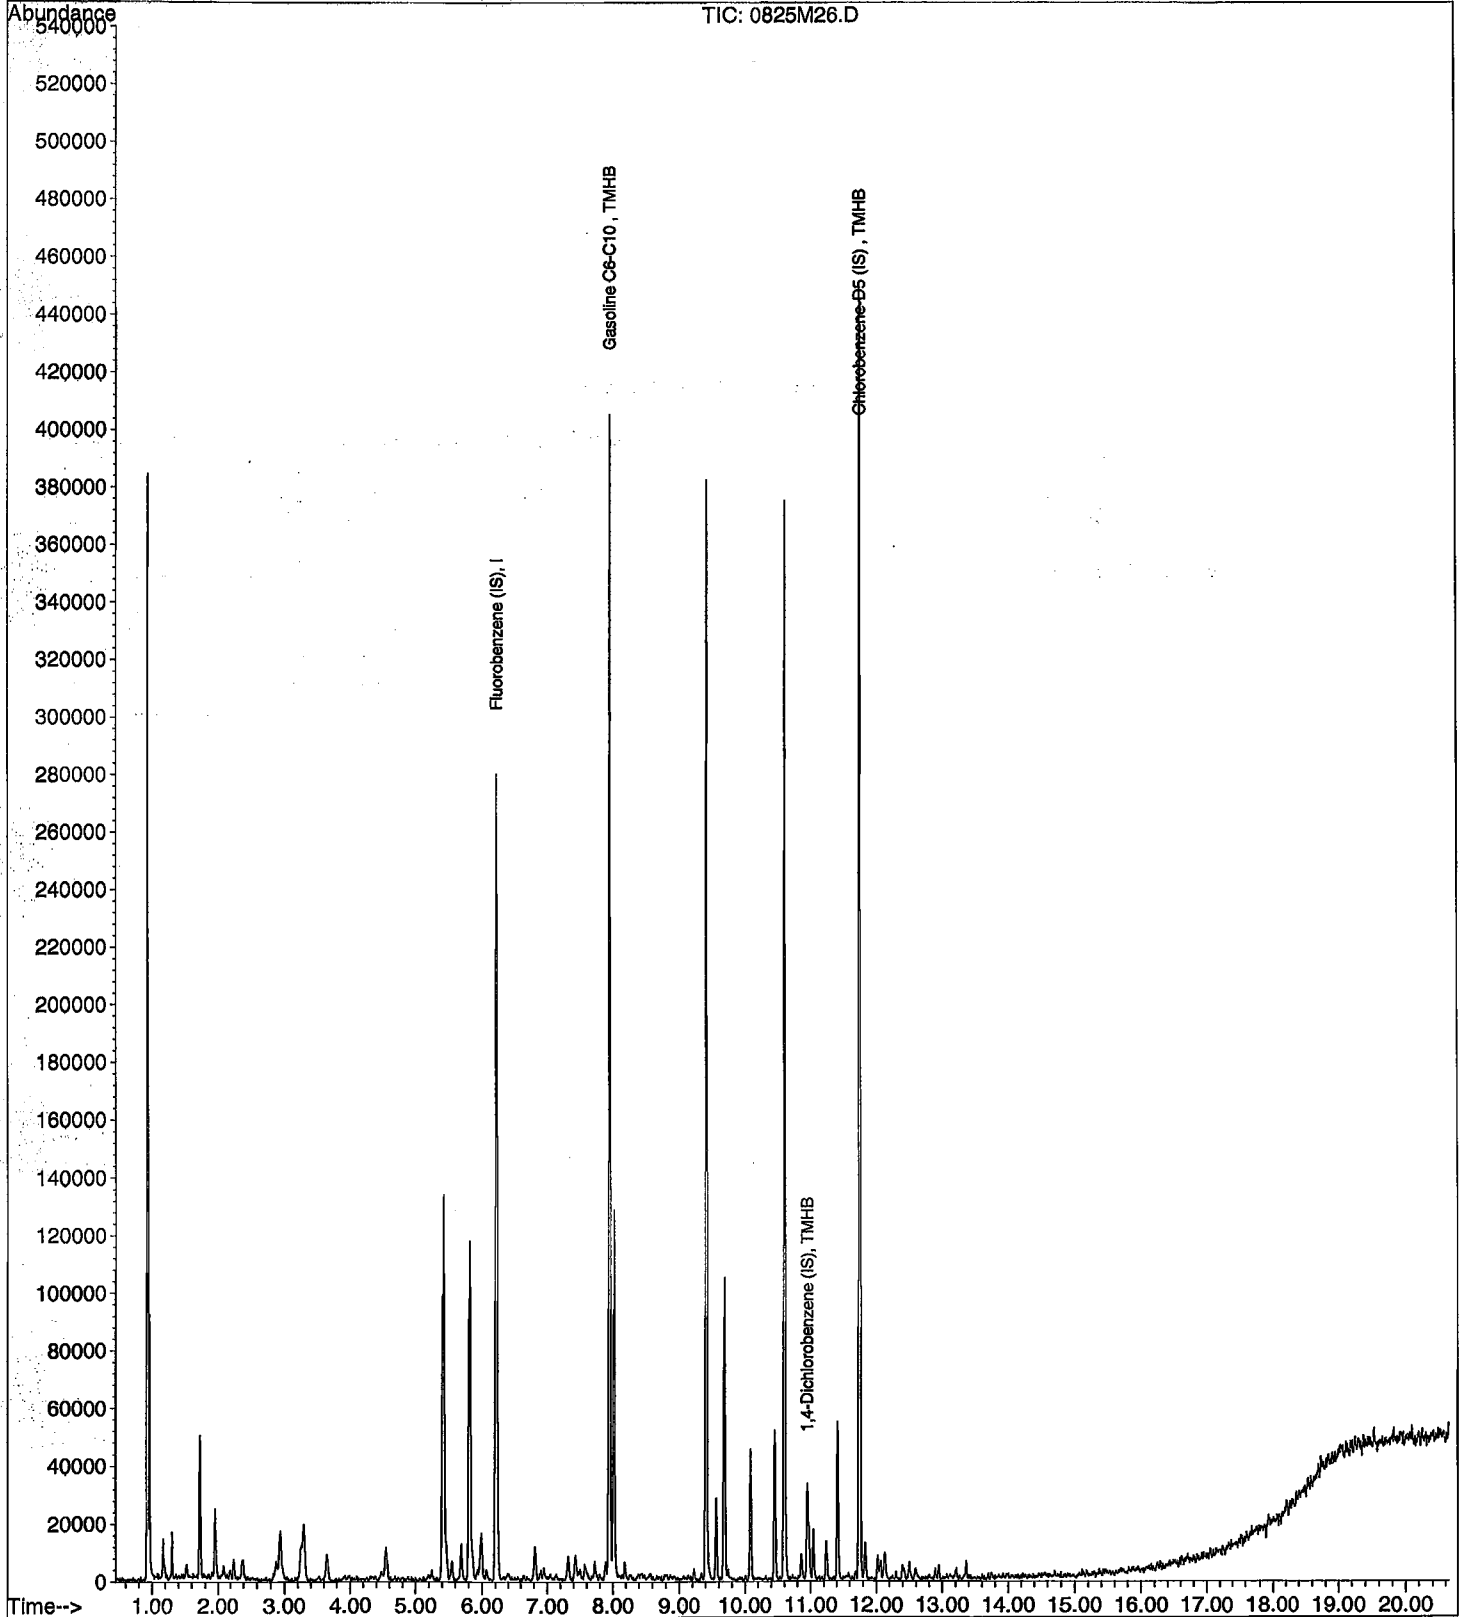

Quantitation Report (Not Reviewed)

Data File : M:\MAX\DATA\210825\0825M27.D
 Acq On : 25 Aug 21 22:14
 Sample : 600ug/L GAS STD 8/25/21
 Misc : IS&S 6/4/21

Vial: 17
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 29 14:41 2021

Quant Results File: MGAS0825.RES

Quant Method : M:\MAX\DATA\210825\MGAS0825.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Thu Aug 26 16:19:36 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260_081021

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.21	TIC	283991	25.00	ppb	0.00
3) Chlorobenzene-D5 (IS)	11.75	TIC	290103m	25.00	ppb	0.00
4) 1,4-Dichlorobenzene (IS)	10.94	TIC	180429m	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Gasoline C6-C10	7.95	TIC	4916556m	442.49	ppb	100

Quantitation Report


Data File : M:\MAX\DATA\210825\0825M27.D
Acq On : 25 Aug 21 22:14
Sample : 600ug/L GAS STD 8/25/21
Misc : IS&S 6/4/21

Vial: 17
Operator: LP,DG,CH
Inst : Max
Multiplr: 1.00

Quant Time: Oct 29 14:41 2021

Quant Results File: MGAS0825.RES

Method : M:\MAX\DATA\211015\MGAS0825.M (RTE Integrator)
Title : METHOD 8260B
Last Update : Thu Aug 26 16:19:36 2021
Response via : Initial Calibration

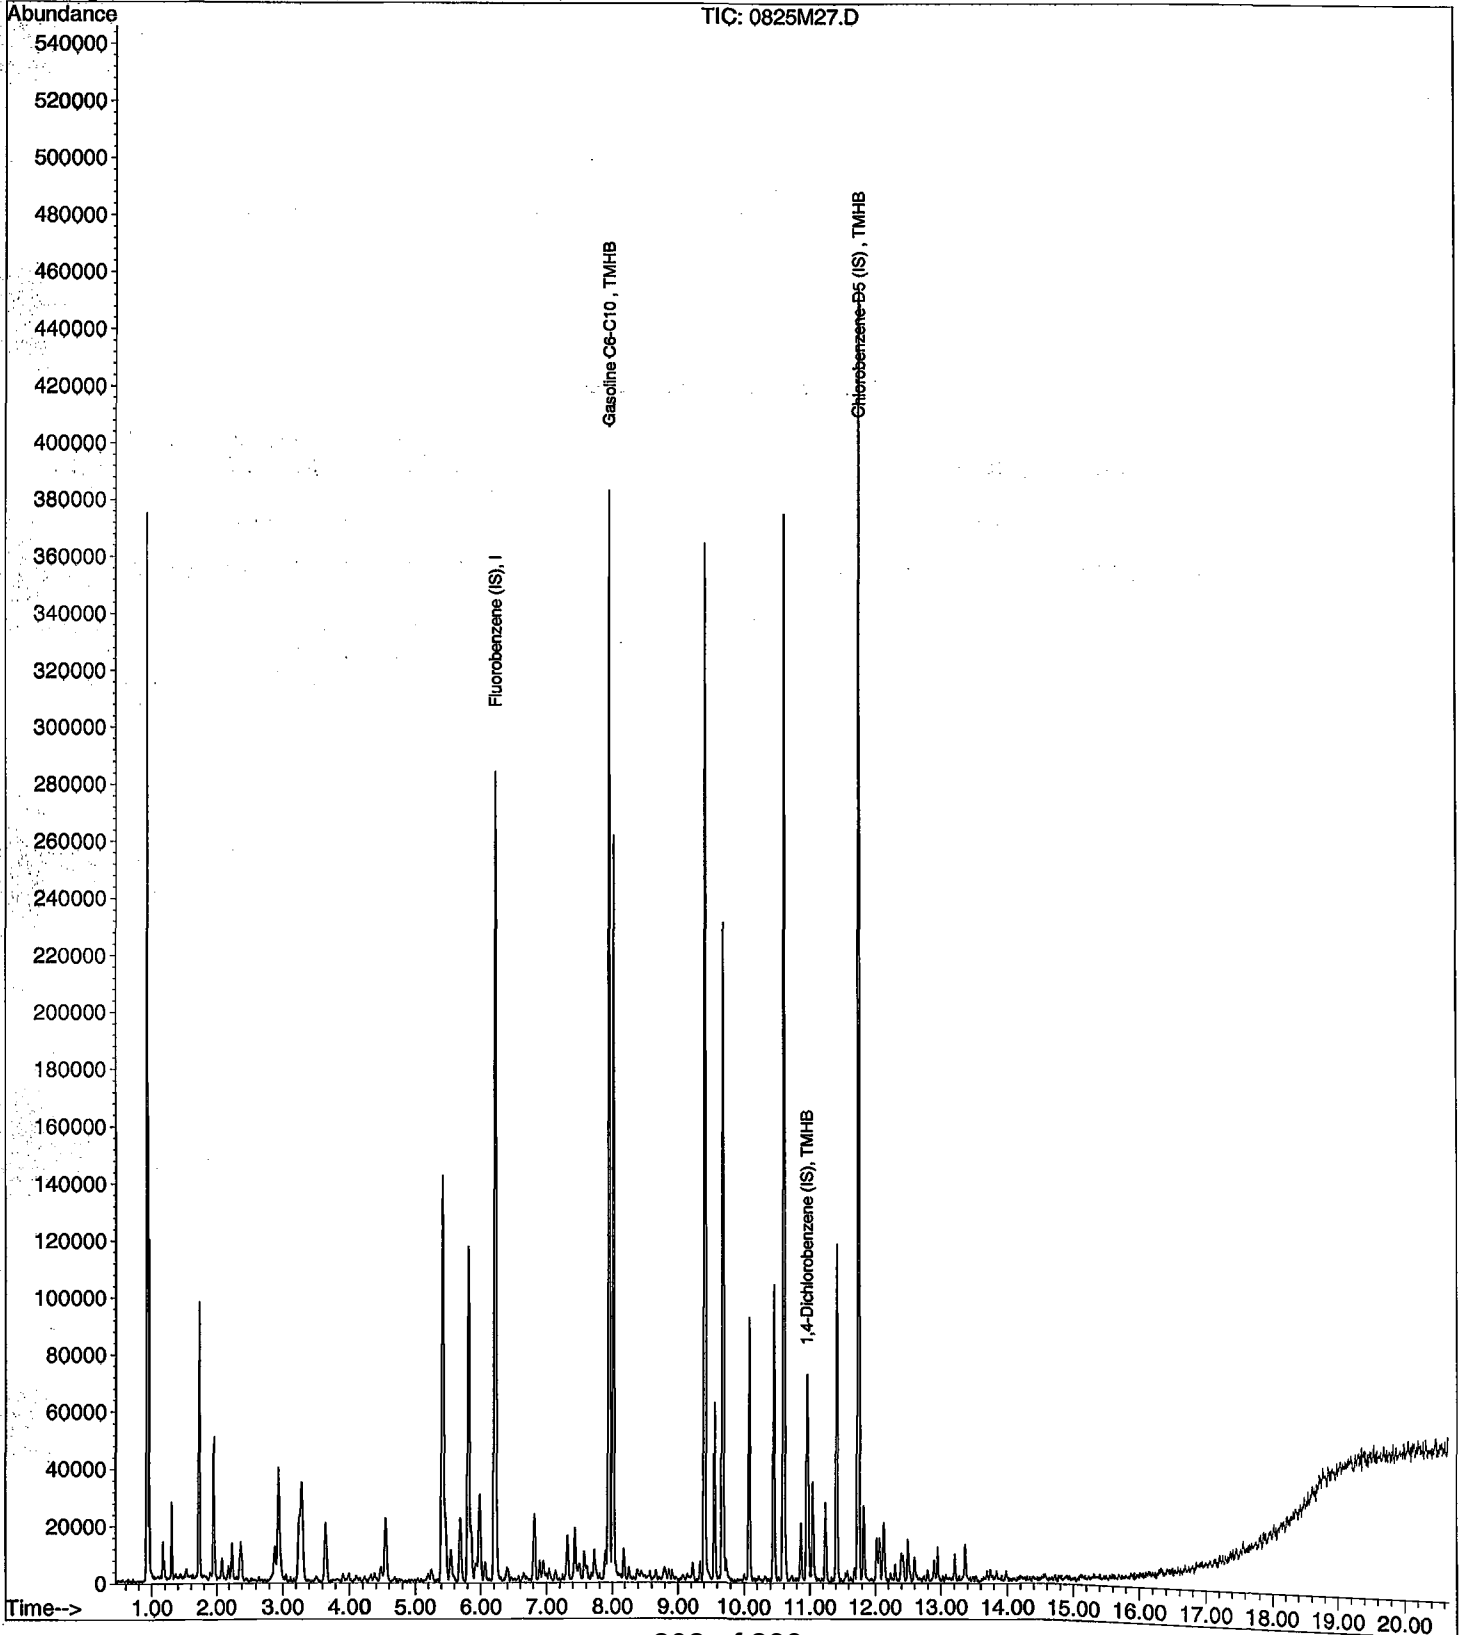

Quantitation Report (Not Reviewed)

Data File : M:\MAX\DATA\210825\0825M28.D
 Acq On : 25 Aug 21 22:42
 Sample : 800ug/L GAS STD 8/25/21
 Misc : IS&S 6/4/21

Vial: 18
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 29 14:41 2021

Quant Results File: MGAS0825.RES

Quant Method : M:\MAX\DATA\210825\MGAS0825.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Thu Aug 26 16:19:36 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260_081021

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.21	TIC	288929	25.00	ppb	0.00
3) Chlorobenzene-D5 (IS)	11.75	TIC	313031m	25.00	ppb	0.00
4) 1,4-Dichlorobenzene (IS)	10.94	TIC	240514m	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Gasoline C6-C10	7.95	TIC	5800436m	628.35	ppb	100

Quantitation Report


Data File : M:\MAX\DATA\210825\0825M28.D
Acq On : 25 Aug 21 22:42
Sample : 800ug/L GAS STD 8/25/21
Misc : IS&S 6/4/21

Vial: 18
Operator: LP,DG,CH
Inst : Max
Multiplr: 1.00

Quant Time: Oct 29 14:41 2021

Quant Results File: MGAS0825.RES

Method : M:\MAX\DATA\211015\MGAS0825.M (RTE Integrator)
Title : METHOD 8260B
Last Update : Thu Aug 26 16:19:36 2021
Response via : Initial Calibration

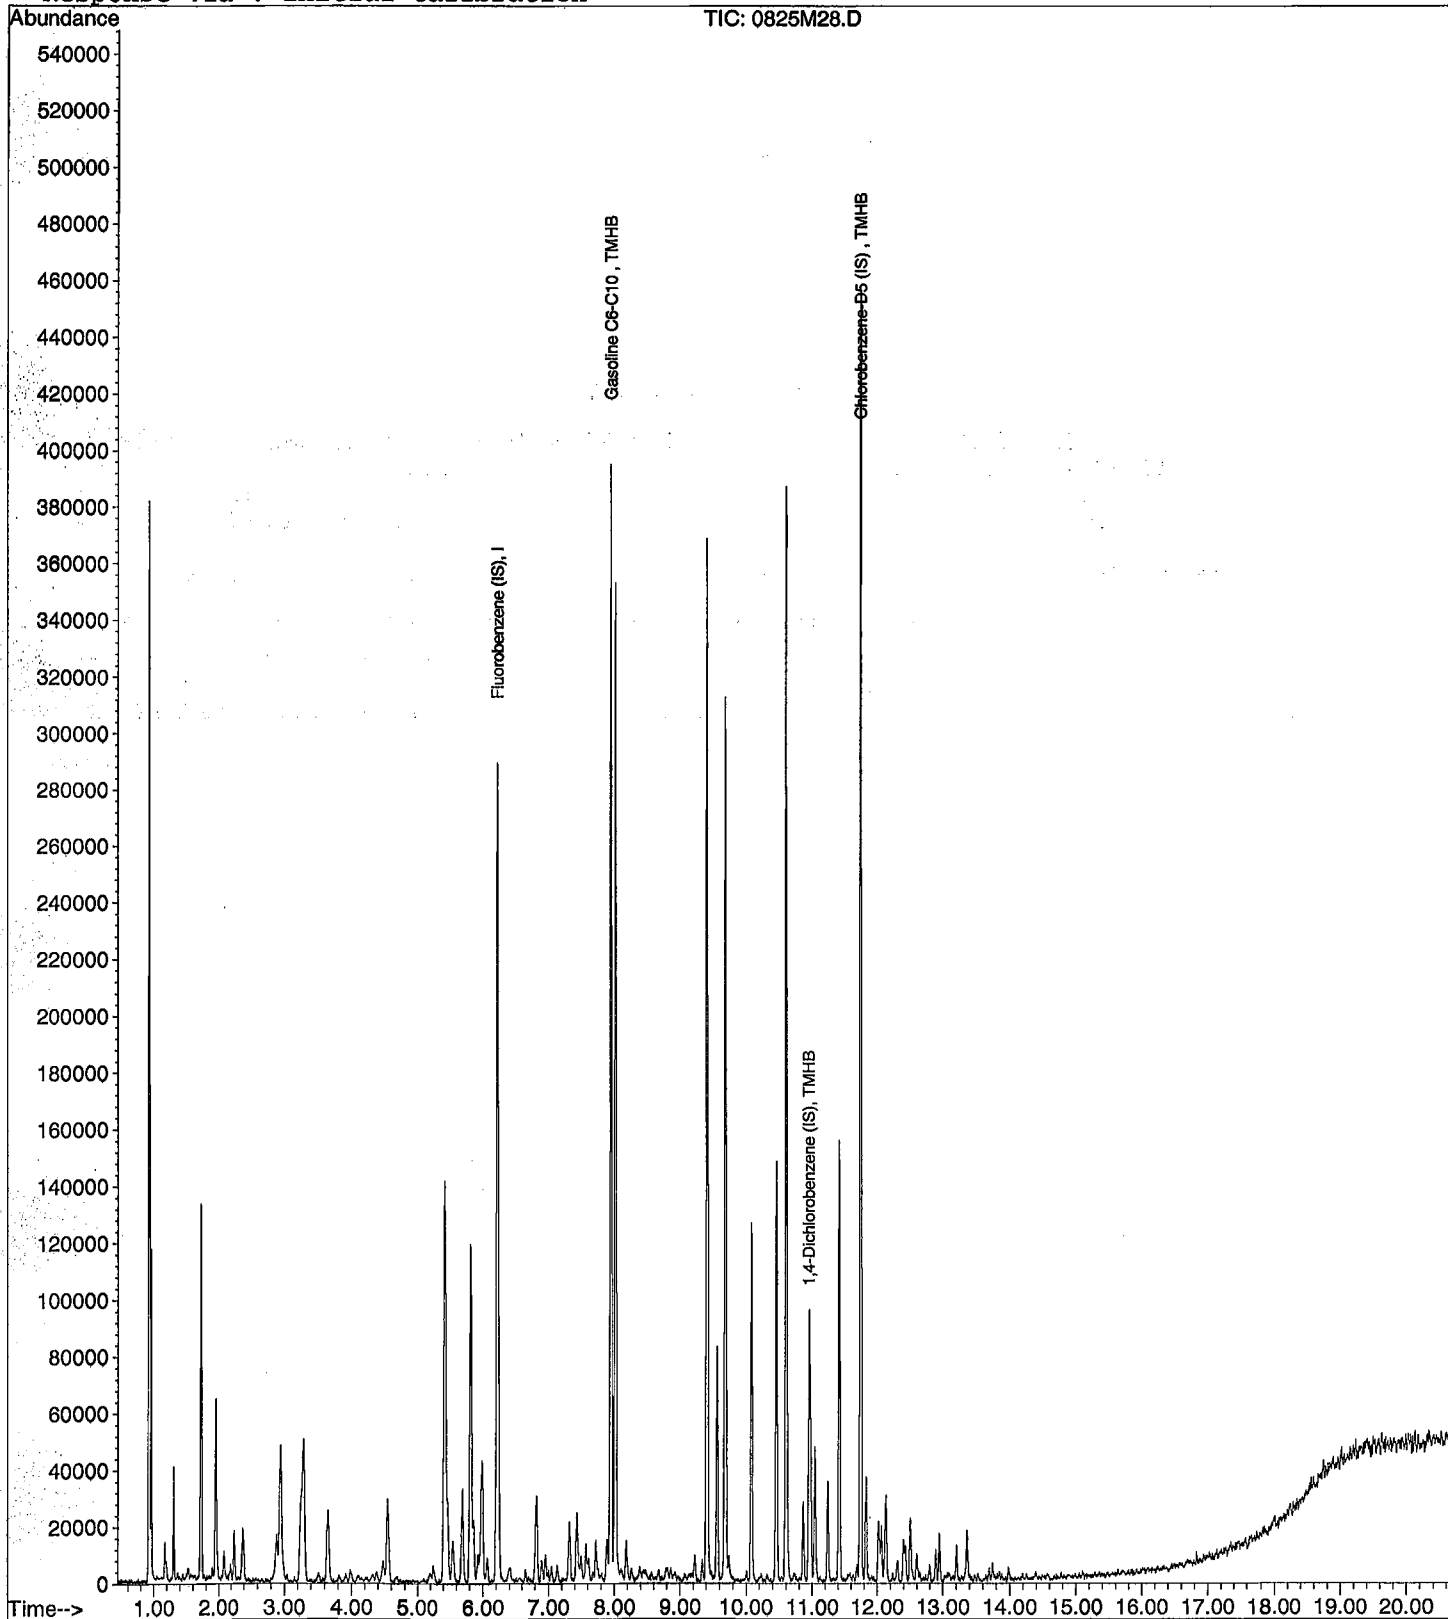

Quantitation Report (Not Reviewed)

Data File : M:\MAX\DATA\210825\0825M29.D
 Acq On : 25 Aug 21 23:10
 Sample : 1000ug/L GAS STD 8/25/21
 Misc : IS&S 6/4/21

Vial: 19
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 29 14:41 2021

Quant Results File: MGAS0825.RES

Quant Method : M:\MAX\DATA\210825\MGAS0825.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Thu Aug 26 16:19:36 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260_081021

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.21	TIC	286598	25.00	ppb	0.00
3) Chlorobenzene-D5 (IS)	11.75	TIC	331346m	25.00	ppb	0.00
4) 1,4-Dichlorobenzene (IS)	10.94	TIC	289883m	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Gasoline C6-C10	7.95	TIC	6556553m	816.79	ppb	100

Quantitation Report


Data File : M:\MAX\DATA\210825\0825M29.D
Acq On : 25 Aug 21 23:10
Sample : 1000ug/L GAS STD 8/25/21
Misc : IS&S 6/4/21

Vial: 19
Operator: LP,DG,CH
Inst : Max
Multiplr: 1.00

Quant Time: Oct 29 14:41 2021

Quant Results File: MGAS0825.RES

Method : M:\MAX\DATA\211015\MGAS0825.M (RTE Integrator)
Title : METHOD 8260B
Last Update : Thu Aug 26 16:19:36 2021
Response via : Initial Calibration

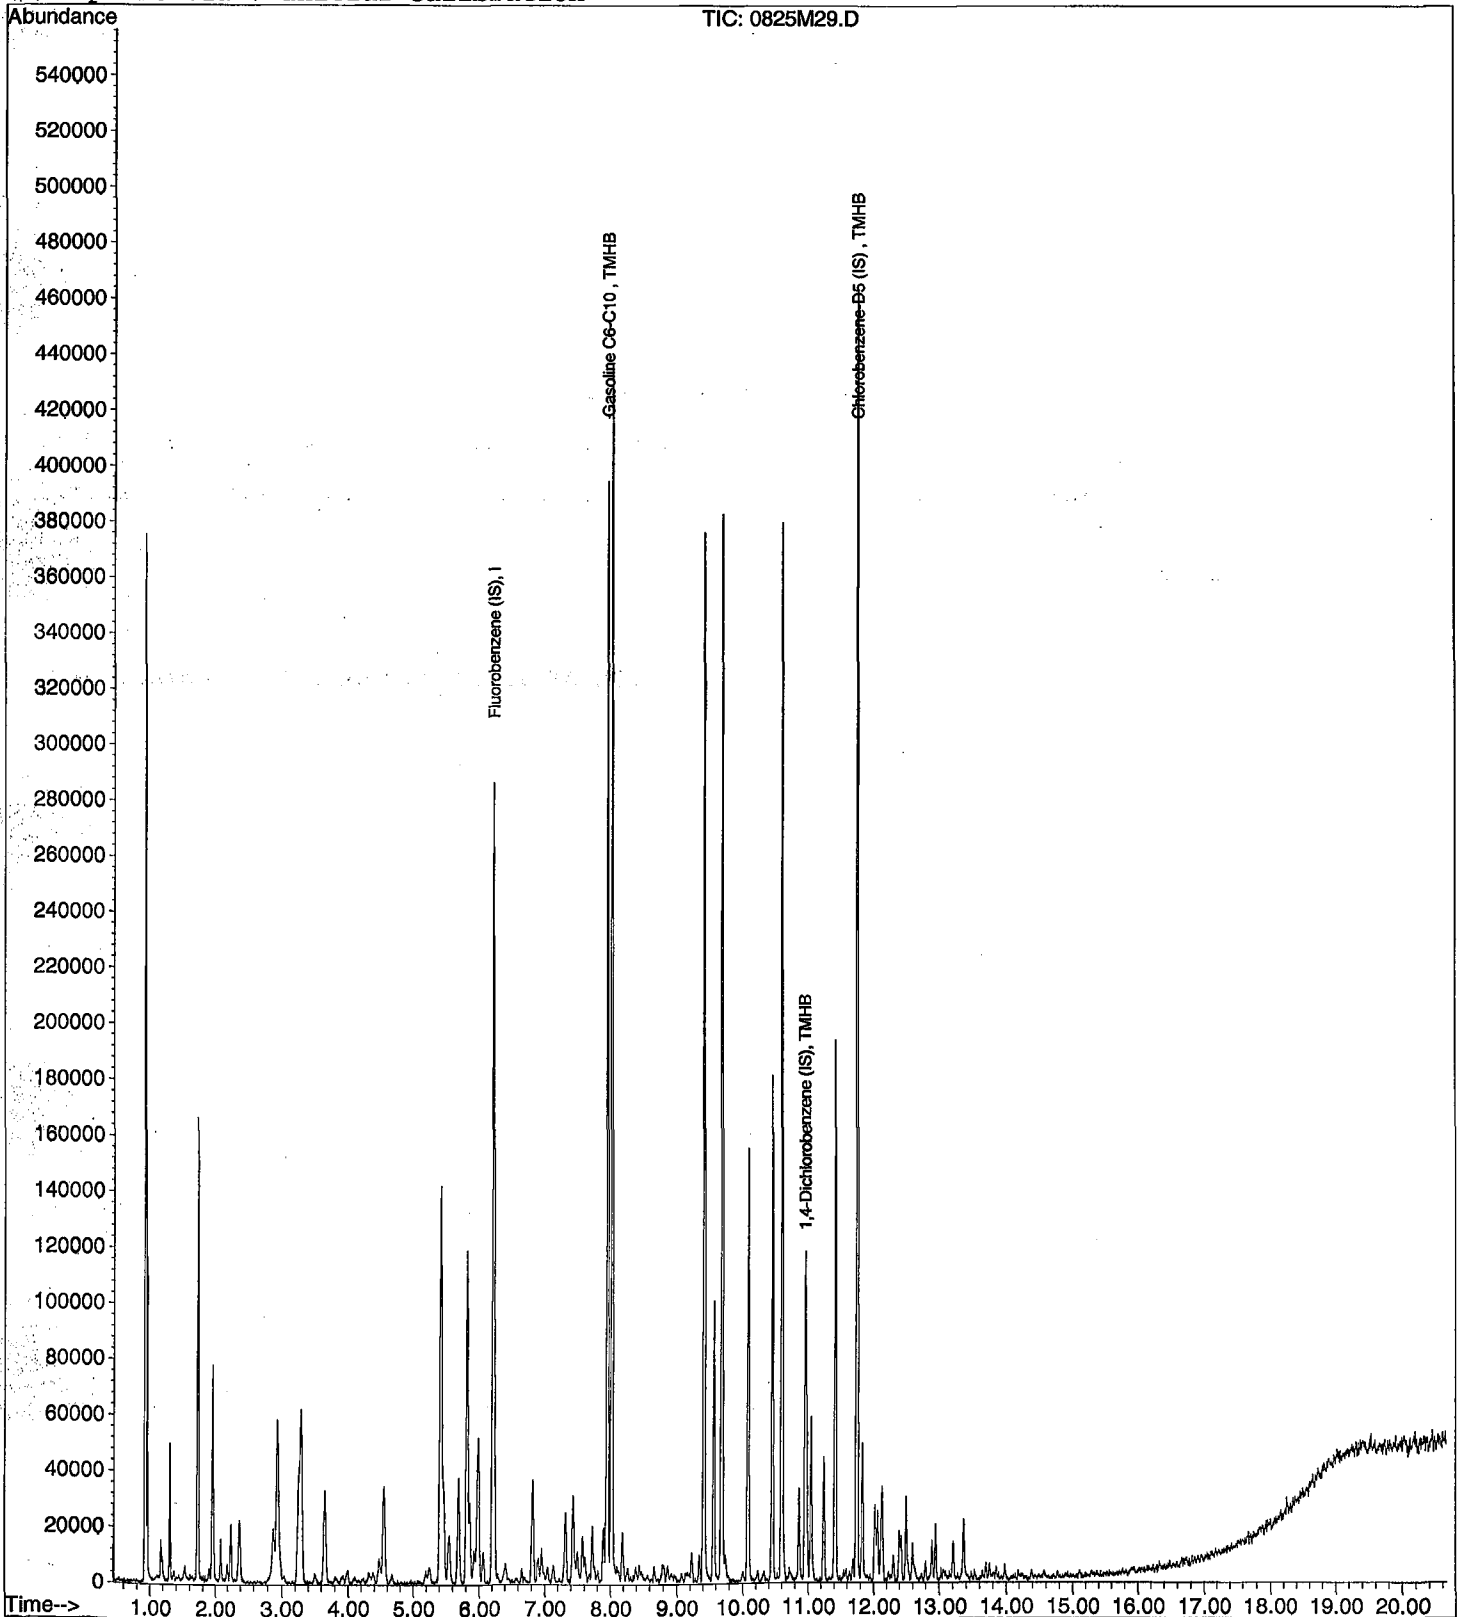

VOLATILE ORGANIC ANALYSIS
VOLATILE ORGANIC COMPOUNDS

Form 7

Second Source Calibration

Lab Name: APPL, Inc.
Case No: _____
Matrix: _____

SDG No: _____
Date Analyzed: 8/26/2021
Instrument: Max
Initial Cal. Date: 8/25/2021
Data File: 0825M31.D

	Compound	MEAN	CCRF	%D	%Drift
1	TMHB Gasoline C6-C10	3.704	1.331	64	TMHBL 17
2					
3					
4					
5					
6					
7					
8					
9					
10					
11					
12					
13					
14					
15					
16					
17					
18					
19					
20					
21					
22					
23					
24					
25					
26					
27					
28					
29					
30					
31					
32					
33					
34					
35					
36					
37					
38					
39					
40	Average			64.0	

Quantitation Report (QT Reviewed)

Data File : M:\MAX\DATA\210825\0825M31.D
 Acq On : 26 Aug 21 00:06
 Sample : (SS) 300ug/L GAS STD 8/25/21
 Misc : IS&S 6/4/21

Vial: 21
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 29 14:57 2021

Quant Results File: MGAS0825.RES

Quant Method : M:\MAX\DATA\210825\MGAS0825.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Thu Aug 26 16:19:36 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260_081021

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.21	TIC	283312	25.00	ppb	0.00
3) Chlorobenzene-D5 (IS)	11.75	TIC	277458m	25.00	ppb	0.00
4) 1,4-Dichlorobenzene (IS)	10.94	TIC	112772m	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Gasoline C6-C10	7.95	TIC	4524430m	352.18	ppb	100

Quantitation Report


Data File : M:\MAX\DATA\210825\0825M31.D
Acq On : 26 Aug 21 00:06
Sample : (SS) 300ug/L GAS STD 8/25/21
Misc : IS&S 6/4/21

Vial: 21
Operator: LP,DG,CH
Inst : Max
Multiplr: 1.00

Quant Time: Oct 29 14:57 2021

Quant Results File: MGAS0825.RES

Method : M:\MAX\DATA\211015\MGAS0825.M (RTE Integrator)
Title : METHOD 8260B
Last Update : Thu Aug 26 16:19:36 2021
Response via : Initial Calibration

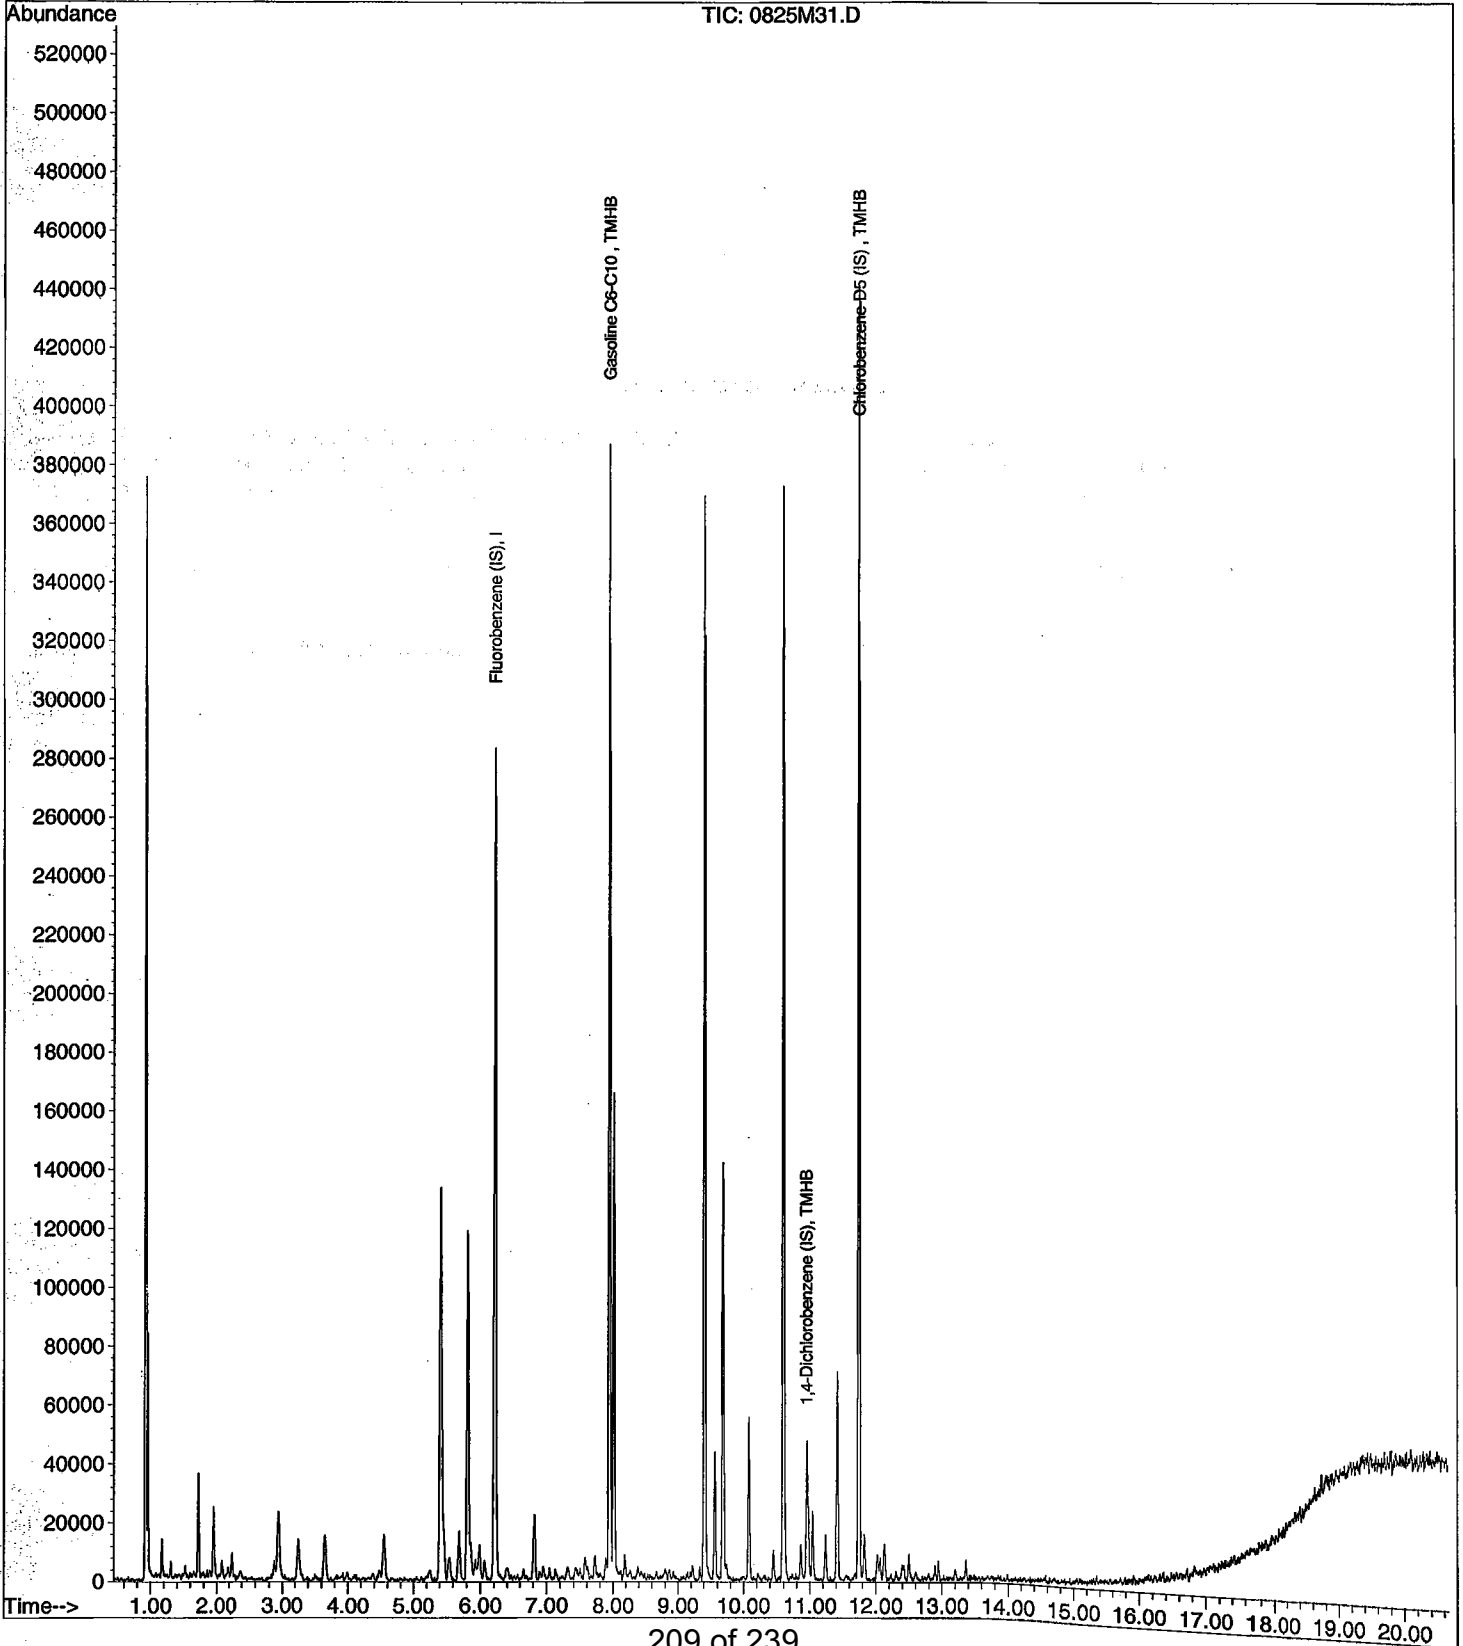

**VOLATILE ORGANIC ANALYSIS
VOLATILE ORGANIC COMPOUNDS**

Form 7

Continuing Calibration

Lab Name: APPL, Inc.
Case No: _____
Matrix: _____

SDG No: _____
Date Analyzed: 10/26/2021
Instrument: Max
Initial Cal. Date: 10/15/2021
Data File: 1026M28.D

	Compound	MEAN	CCRF	%D	%Drift	
1	Fluorobenzene (IS)	ISTD				
2	TMHB Gasoline C6-C10	3.704	1.331	64	TMHBL	17
3	TMHB Chlorobenzene-D5 (IS)	ISTD			TMHB	
4	TMHB 1,4-Dichlorobenzene (IS)	ISTD			TMHB	
5						
6						
7						
8						
9						
10						
11						
12						
13						
14						
15						
16						
17						
18						
19						
20						
21						
22						
23						
24						
25						
26						
27						
28						
29						
30						
31						
32						
33						
34						
35						
36						
37						
38						
39						
40						

Average

64.0

Quantitation Report (QT Reviewed)

Data File : M:\MAX\DATA\211015\1026M28.D
 Acq On : 26 Oct 21 21:55
 Sample : 211026B CCV 300ug/L
 Misc : IS&S 8/4/21

Vial: 28
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 28 14:43 2021

Quant Results File: MGAS0825.RES

Quant Method : M:\MAX\DATA\210825\MGAS0825.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Thu Aug 26 16:19:36 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.37	TIC	421508	25.00	ppb	0.16
3) Chlorobenzene-D5 (IS)	11.75	TIC	1180010m	25.00	ppb	0.00
4) 1,4-Dichlorobenzene (IS)	10.94	TIC	118167m	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Gasoline C6-C10	8.08	TIC	6729880m	351.94	ppb	100

Quantitation Report (Not Reviewed)

Data File : M:\MAX\DATA\211015\1026M28.D
 Acq On : 26 Oct 21 21:55
 Sample : 211026B CCV 300ug/L
 Misc : IS&S 8/4/21

Vial: 28
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Nov 30 12:58 2021

Quant Results File: M0825SUR.RES

Quant Method : M:\MAX\DATA\210825\M0825SUR.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Thu Aug 26 11:16:48 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.37	96	351549	25.00	ppb	0.16
4) Chlorobenzene-D5 (IS)	9.53	117	334953	25.00	ppb	0.12
7) 1,4-Dichlorobenzene-D (IS)	11.84	152	221397	25.00	ppb	0.10
System Monitoring Compounds						
2) Dibromofluoromethane(S)	5.59	111	118199	27.88	ppb	0.18
Spiked Amount	25.000		Recovery	=	111.516%	
3) 1,2-DCA-D4(S)	5.98	65	78160	28.05	ppb	0.17
Spiked Amount	25.000		Recovery	=	112.212%	
5) Toluene-D8(S)	8.08	98	386568	24.61	ppb	0.13
Spiked Amount	25.000		Recovery	=	98.444%	
6) 4-Bromofluorobenzene(S)	10.70	95	156655	25.56	ppb	0.11
Spiked Amount	25.000		Recovery	=	102.252%	

Target Compounds

Qvalue

Quantitation Report


Data File : M:\MAX\DATA\211015\1026M28.D
Acq On : 26 Oct 21 21:55
Sample : 211026B CCV 300ug/L
Misc : IS&S 8/4/21

Vial: 28
Operator: LP,DG,CH
Inst : Max
Multiplr: 1.00

Quant Time: Oct 28 14:43 2021

Quant Results File: MGAS0825.RES

Method : M:\MAX\DATA\211015\MGAS0825.M (RTE Integrator)
Title : METHOD 8260B
Last Update : Thu Aug 26 16:19:36 2021
Response via : Initial Calibration

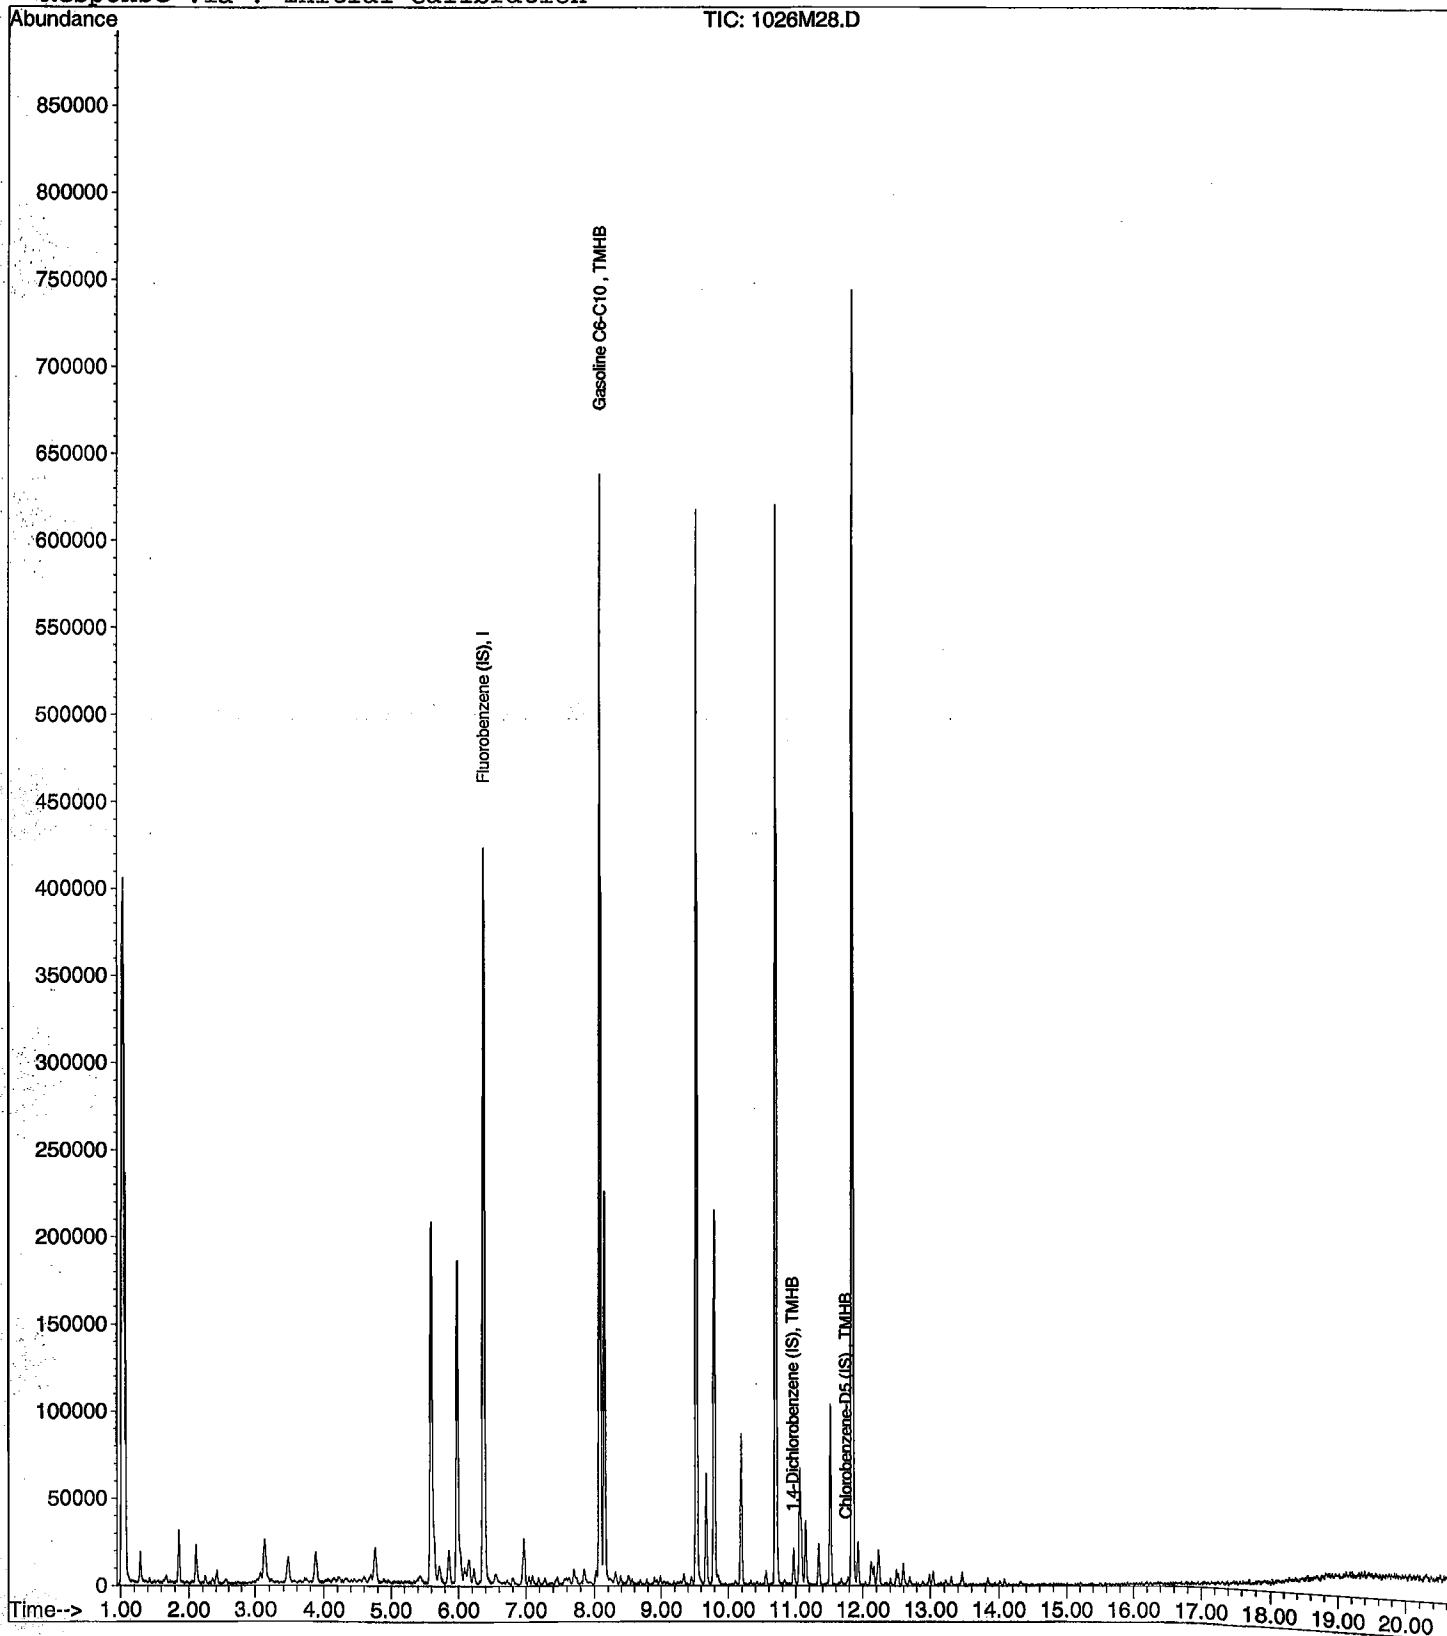

VOLATILE ORGANIC ANALYSIS
VOLATILE ORGANIC COMPOUNDS

Form 7

Continuing Calibration

Lab Name: APPL, Inc.

SDG No: _____

Case No: _____

Date Analyzed: 10/27/2021

Matrix: _____

Instrument: Max

Initial Cal. Date: 8/25/2021

Data File: 1026M46.D

		Compound	MEAN	CCRF	%D		%Drift
1	I	Fluorobenzene (IS)	ISTD			I	
2	TMHB	Gasoline C6-C10	3.704	1.290	65	TMHBL	6.5
3	TMHB	Chlorobenzene-D5 (IS)	ISTD			TMHB	
4	TMHB	1,4-Dichlorobenzene (IS)	ISTD			TMHB	
5							
6							
7							
8							
9							
10							
11							
12							
13							
14							
15							
16							
17							
18							
19							
20							
21							
22							
23							
24							
25							
26							
27							
28							
29							
30							
31							
32							
33							
34							
35							
36							
37							
38							
39							
40							

Average

65.0

Data File : M:\MAX\DATA\211015\1026M46.D
 Acq On : 27 Oct 21 6:23
 Sample : Ending CCV 300ug/L 10/26/21
 Misc : IS&S 8/4/21

Vial: 46
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 28 14:45 2021

Quant Results File: MGAS0825.RES

Quant Method : M:\MAX\DATA\210825\MGAS0825.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Thu Aug 26 16:19:36 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.37	TIC	470524	25.00	ppb	0.16
3) Chlorobenzene-D5 (IS)	11.75	TIC	1183520m	25.00	ppb	0.00
4) 1,4-Dichlorobenzene (IS)	10.94	TIC	119761m	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Gasoline C6-C10	8.07	TIC	7285476m	319.49	ppb	100

Quantitation Report


Data File : M:\MAX\DATA\211015\1026M46.D
Acq On : 27 Oct 21 6:23
Sample : Ending CCV 300ug/L 10/26/21
Misc : IS&S 8/4/21

Vial: 46
Operator: LP,DG,CH
Inst : Max
Multiplr: 1.00

Quant Time: Oct 28 14:45 2021

Quant Results File: MGAS0825.RES

Method : M:\MAX\DATA\211015\MGAS0825.M (RTE Integrator)
Title : METHOD 8260B
Last Update : Thu Aug 26 16:19:36 2021
Response via : Initial Calibration

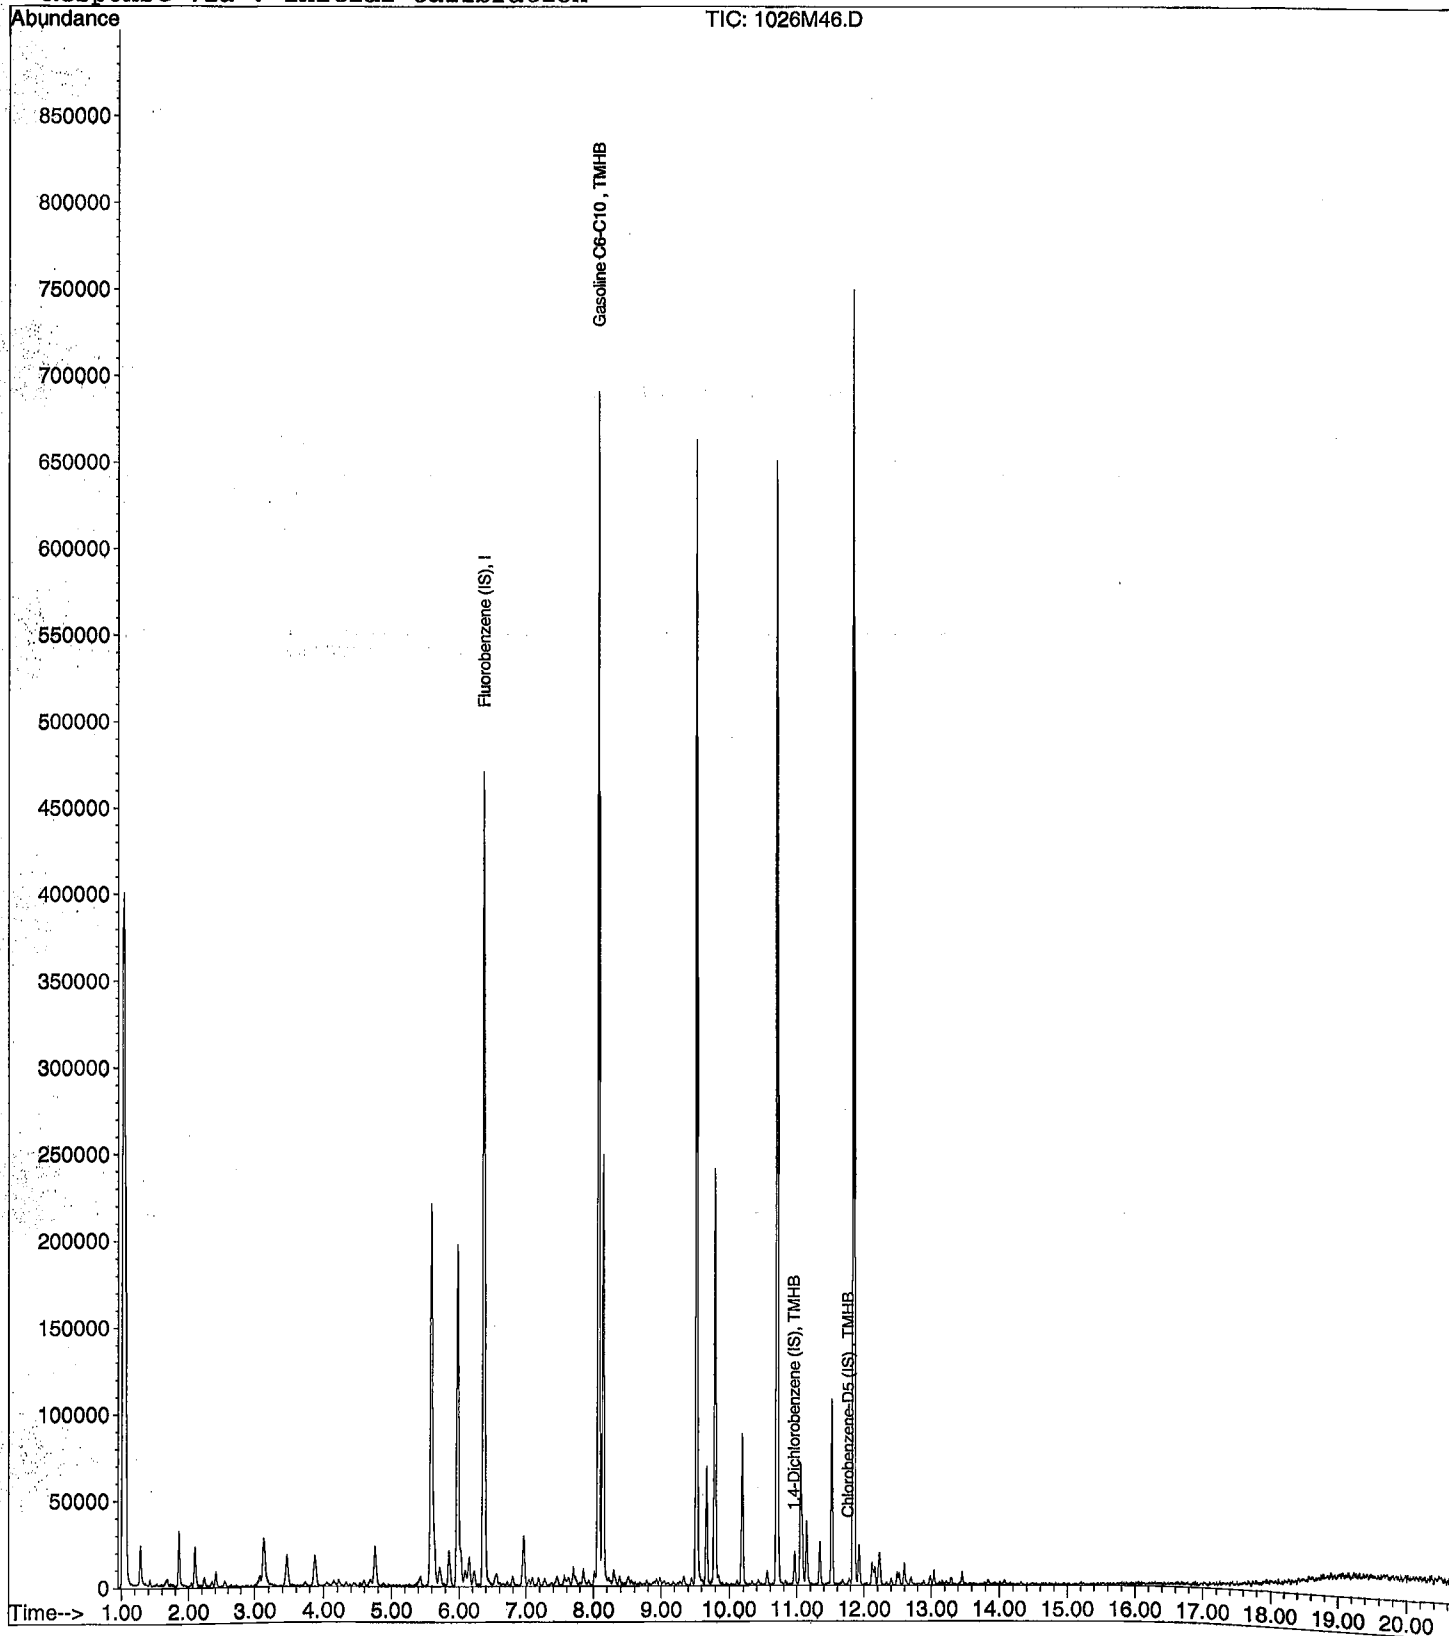

ORGANICS
Raw Data

Quantitation Report (QT Reviewed)

Data File : M:\MAX\DATA\211015\1026M35.D
 Acq On : 27 Oct 21 1:13
 Sample : BA43836W01
 Misc : IS&S 8/4/21

Vial: 35
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Nov 30 12:55 2021

Quant Results File: MGAS0825.RES

Quant Method : M:\MAX\DATA\211015\MGAS0825.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Thu Aug 26 16:19:36 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.37	TIC	431207	25.00	ppb	0.16
3) Chlorobenzene-D5 (IS)	11.75	TIC	1101207m	25.00	ppb	0.00
4) 1,4-Dichlorobenzene (IS)	10.94	TIC	8454m	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds

Qvalue

Data File : M:\MAX\DATA\211015\1026M35.D
 Acq On : 27 Oct 21 1:13
 Sample : BA43836W01
 Misc : IS&S 8/4/21
 MS Integration Params: LSCINT.P
 Quant Time: Nov 30 13:16 2021

Vial: 35
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00000

Quant Results File: M0825SUR.RES

Quant Method : M:\MAX\DATA\210825\M0825SUR.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Thu Aug 26 11:16:48 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.37	96	368836	25.00	ppb	0.16
4) Chlorobenzene-D5 (IS)	9.53	117	343273	25.00	ppb	0.12
7) 1,4-Dichlorobenzene-D (IS)	11.85	152	205124	25.00	ppb	0.10

System Monitoring Compounds						
2) Dibromofluoromethane(S)	5.59	111	122341	27.50	ppb	0.18
Spiked Amount 25.000			Recovery =			110.016%
3) 1,2-DCA-D4(S)	5.98	65	82080	28.08	ppb	0.16
Spiked Amount 25.000			Recovery =			112.316%
5) Toluene-D8(S)	8.08	98	394249	24.49	ppb	0.13
Spiked Amount 25.000			Recovery =			97.968%
6) 4-Bromofluorobenzene(S)	10.70	95	154312	24.57	ppb	0.11
Spiked Amount 25.000			Recovery =			98.284%

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration
 1026M35.D M0825SUR.M Tue Nov 30 13:16:33 2021

Quantitation Report


Data File : M:\MAX\DATA\211015\1026M35.D
Acq On : 27 Oct 21 1:13
Sample : BA43836W01
Misc : IS&S 8/4/21

Vial: 35
Operator: LP,DG,CH
Inst : Max
Multiplr: 1.00

Quant Time: Nov 30 12:55 2021

Quant Results File: MGAS0825.RES

Method : M:\MAX\DATA\211015\MGAS0825.M (RTE Integrator)
Title : METHOD 8260B
Last Update : Thu Aug 26 16:19:36 2021
Response via : Initial Calibration

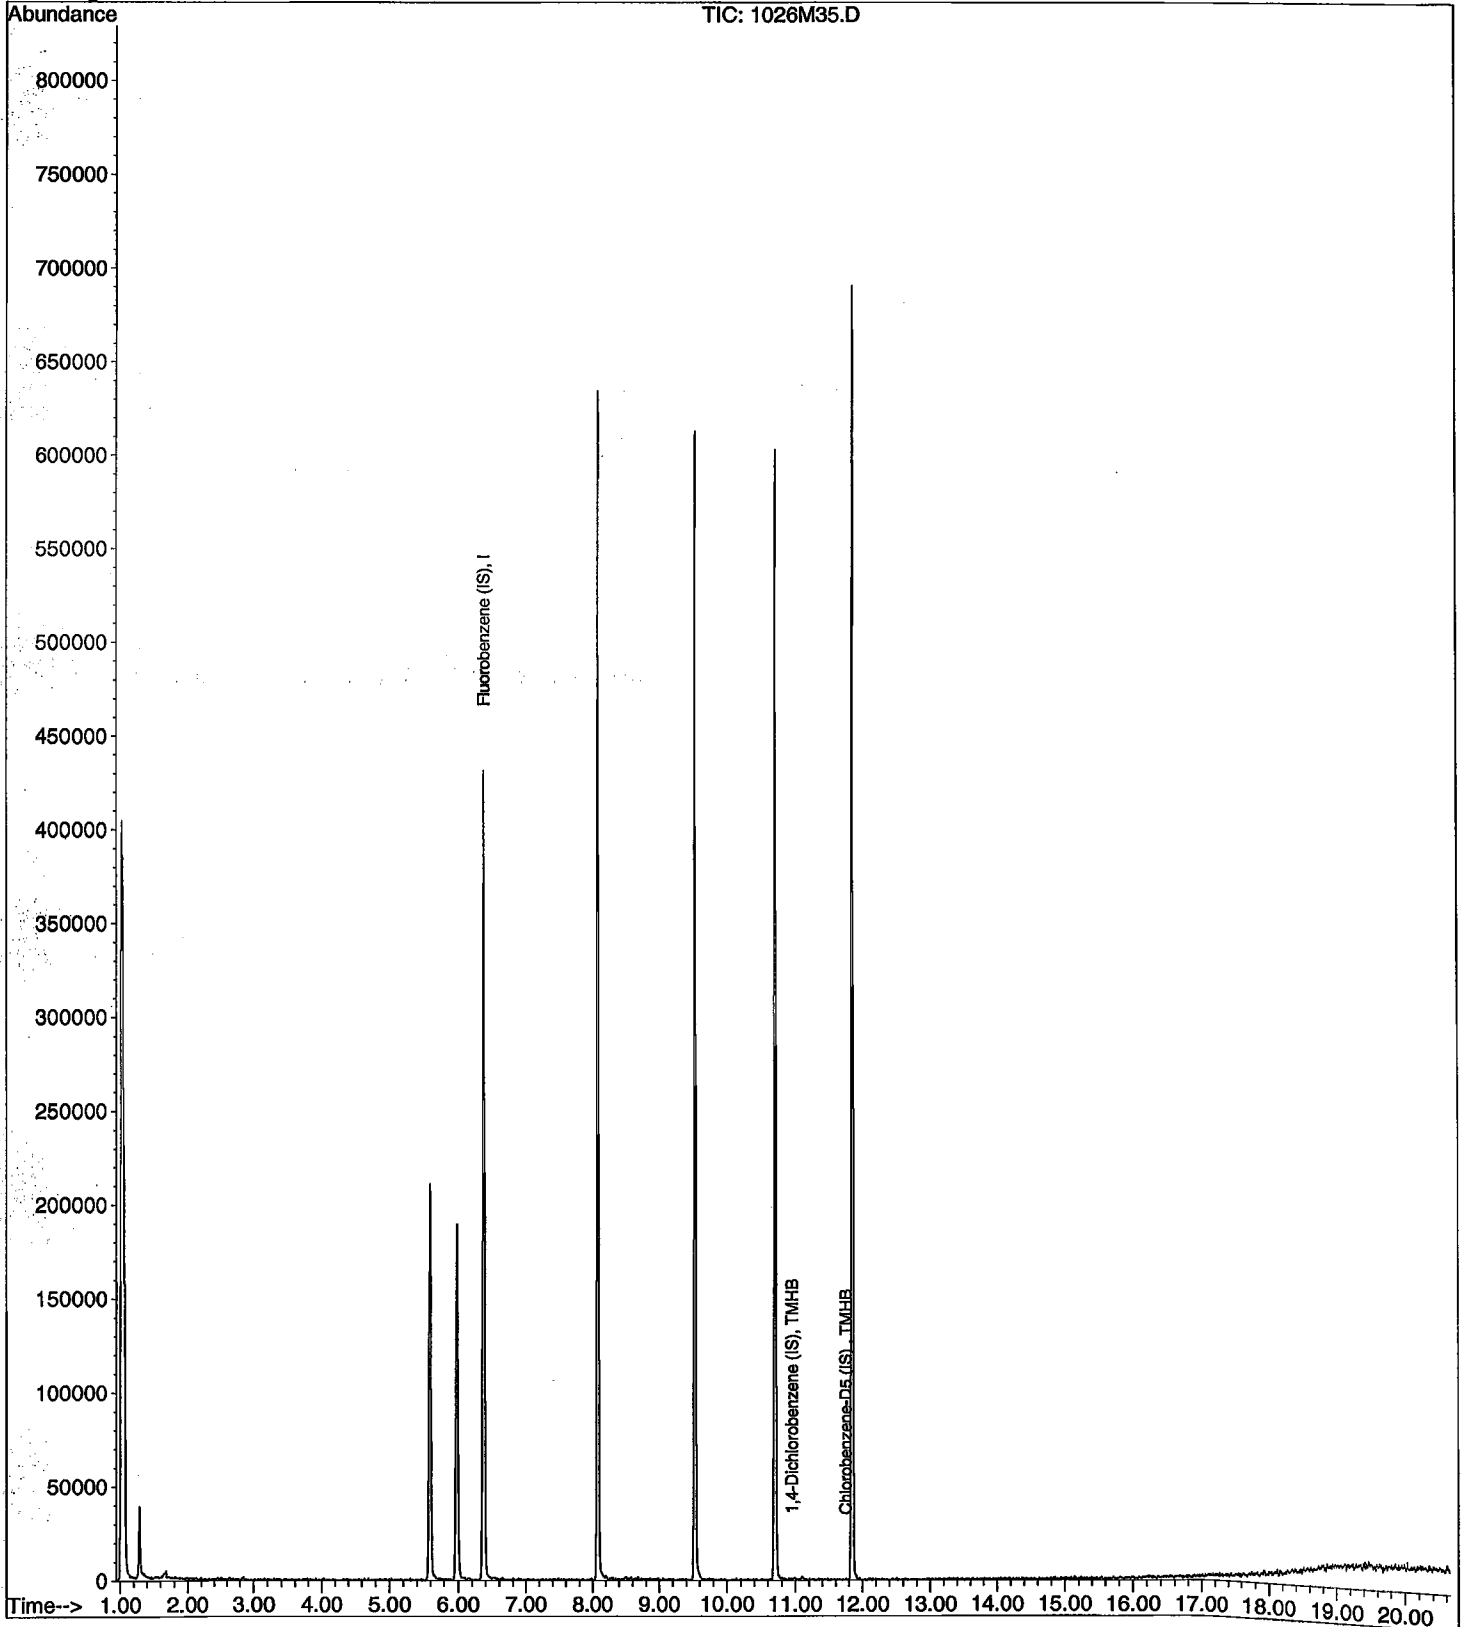

Quantitation Report (QT Reviewed)

Data File : M:\MAX\DATA\211015\1026M36.D
 Acq On : 27 Oct 21 1:41
 Sample : BA43837W01
 Misc : IS&S 8/4/21

Vial: 36
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Nov 30 12:55 2021

Quant Results File: MGAS0825.RES

Quant Method : M:\MAX\DATA\211015\MGAS0825.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Thu Aug 26 16:19:36 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.37	TIC	446330	25.00	ppb	0.16
3) Chlorobenzene-D5 (IS)	11.75	TIC	1116426m	25.00	ppb	0.00
4) 1,4-Dichlorobenzene (IS)	10.94	TIC	6504m	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds

Qvalue

Data File : M:\MAX\DATA\211015\1026M36.D
 Acq On : 27 Oct 21 1:41
 Sample : BA43837W01
 Misc : IS&S 8/4/21
 MS Integration Params: LSCINT.P
 Quant Time: Nov 30 13:16 2021

Vial: 36
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00000

Quant Results File: M0825SUR.RES

Quant Method : M:\MAX\DATA\210825\M0825SUR.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Thu Aug 26 11:16:48 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.37	96	377483	25.00	ppb	0.16
4) Chlorobenzene-D5 (IS)	9.53	117	341211	25.00	ppb	0.12
7) 1,4-Dichlorobenzene-D (IS)	11.84	152	210844	25.00	ppb	0.10

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev (Min)
2) Dibromofluoromethane(S)	5.59	111	121910	26.78	ppb	0.17
Spiked Amount 25.000			Recovery =	107.116%		
3) 1,2-DCA-D4(S)	5.98	65	82168	27.47	ppb	0.17
Spiked Amount 25.000			Recovery =	109.864%		
5) Toluene-D8(S)	8.08	98	401448	25.09	ppb	0.13
Spiked Amount 25.000			Recovery =	100.356%		
6) 4-Bromofluorobenzene(S)	10.70	95	152105	24.37	ppb	0.11
Spiked Amount 25.000			Recovery =	97.464%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration
 1026M36.D M0825SUR.M Tue Nov 30 13:16:46 2021

Quantitation Report


Data File : M:\MAX\DATA\211015\1026M36.D
Acq On : 27 Oct 21 1:41
Sample : BA43837W01
Misc : IS&S 8/4/21

Vial: 36
Operator: LP,DG,CH
Inst : Max
Multiplr: 1.00

Quant Time: Nov 30 12:55 2021

Quant Results File: MGAS0825.RES

Method : M:\MAX\DATA\211015\MGAS0825.M (RTE Integrator)
Title : METHOD 8260B
Last Update : Thu Aug 26 16:19:36 2021
Response via : Initial Calibration

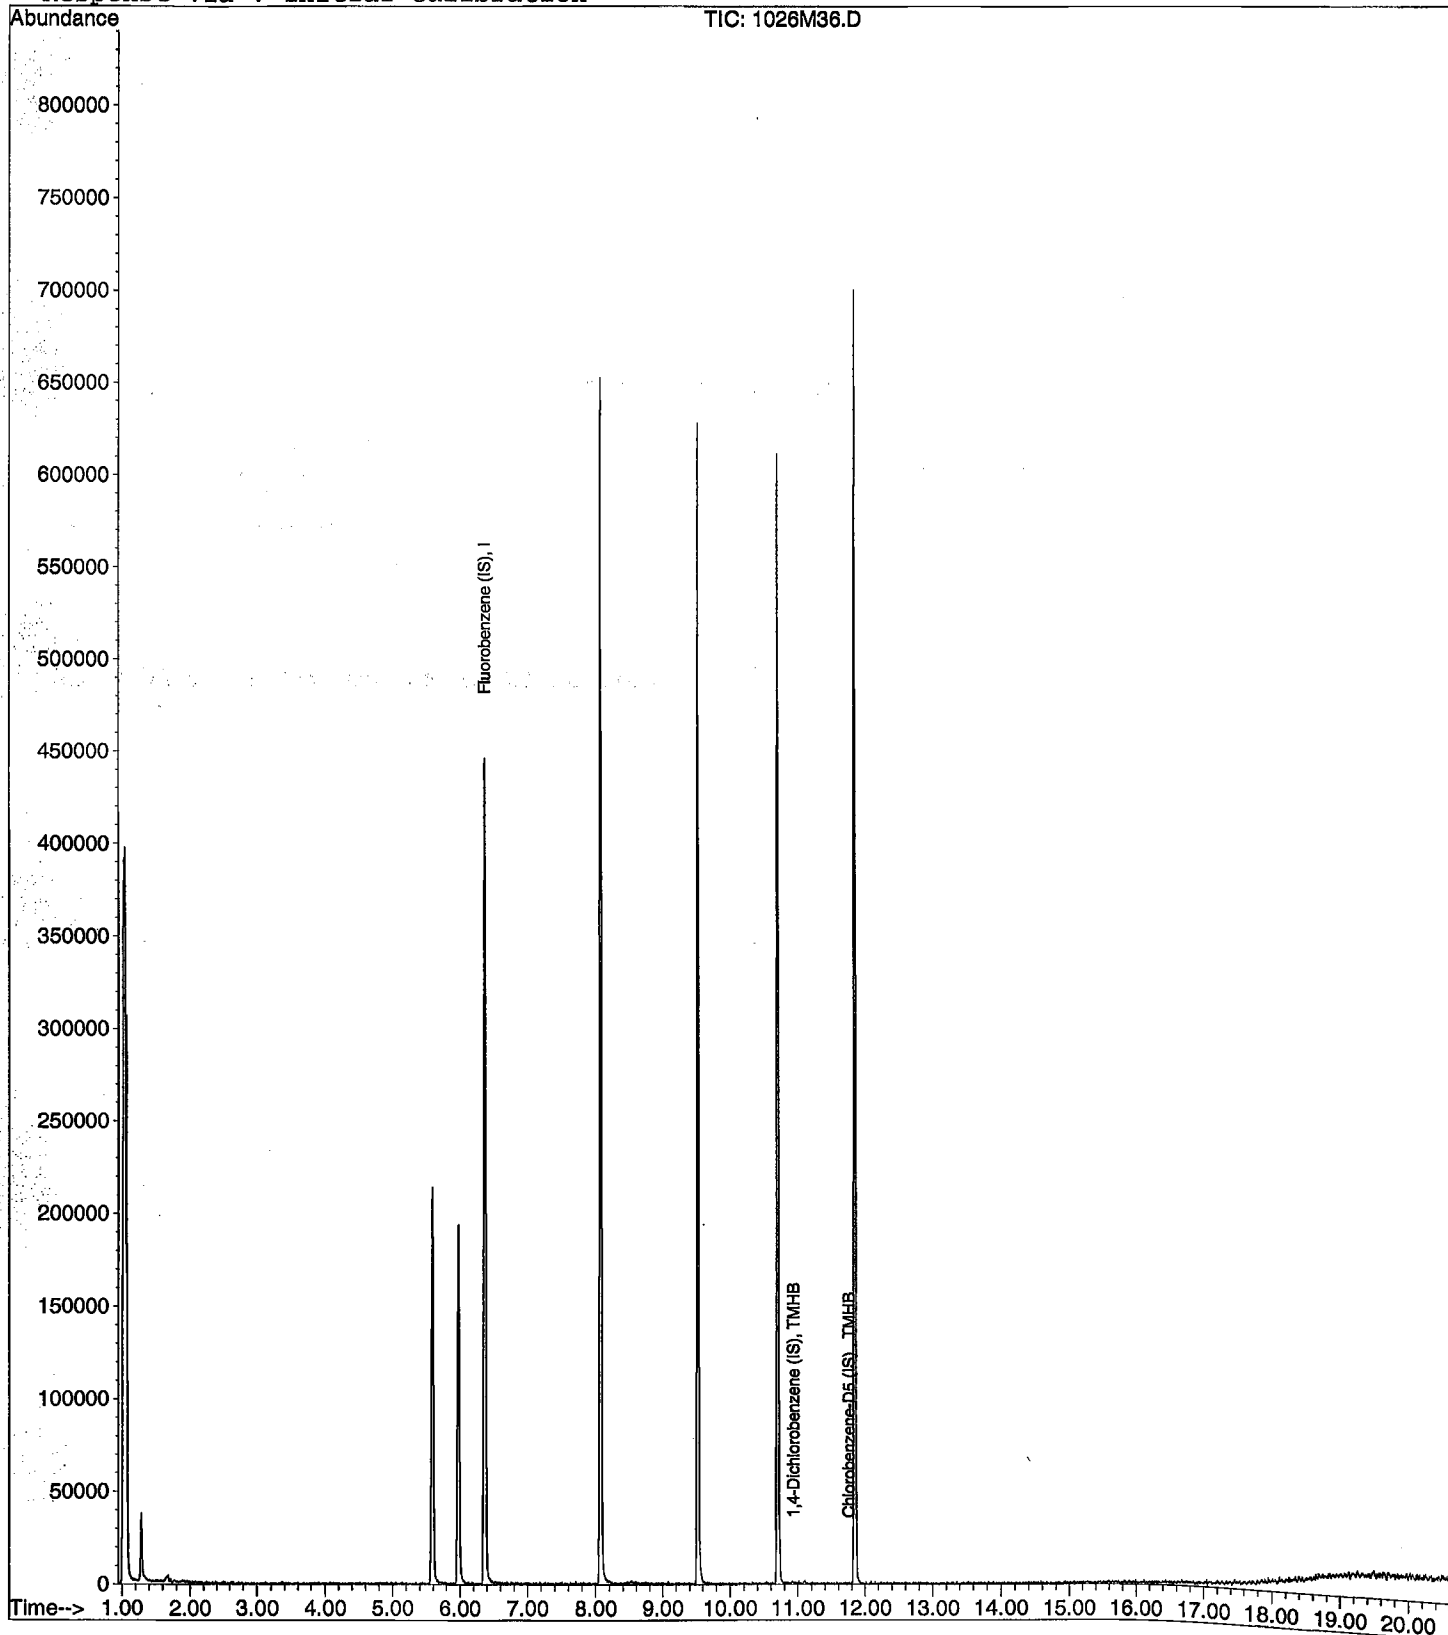

Quantitation Report (QT Reviewed)

Data File : M:\MAX\DATA\211015\1026M31.D
 Acq On : 26 Oct 21 23:20
 Sample : 211026B BLK
 Misc : IS&S 8/4/21

Vial: 31
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Nov 30 13:11 2021

Quant Results File: MGAS0825.RES

Quant Method : M:\MAX\DATA\210825\MGAS0825.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Thu Aug 26 16:19:36 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.37	TIC	454647	25.00	ppb	0.16
3) Chlorobenzene-D5 (IS)	11.75	TIC	1149629m	25.00	ppb	0.00
4) 1,4-Dichlorobenzene (IS)	10.94	TIC	10149m	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds Qvalue

Quantitation Report (Not Reviewed)

Data File : M:\MAX\DATA\211015\1026M31.D
 Acq On : 26 Oct 21 23:20
 Sample : 211026B BLK
 Misc : IS&S 8/4/21

Vial: 31
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Nov 30 12:58 2021

Quant Results File: M0825SUR.RES

Quant Method : M:\MAX\DATA\210825\M0825SUR.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Thu Aug 26 11:16:48 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.37	96	385706	25.00	ppb	0.16
4) Chlorobenzene-D5 (IS)	9.53	117	350438	25.00	ppb	0.11
7) 1,4-Dichlorobenzene-D (IS)	11.85	152	212898	25.00	ppb	0.10
System Monitoring Compounds						
2) Dibromofluoromethane(S)	5.59	111	122799	26.40	ppb	0.17
Spiked Amount	25.000		Recovery	=	105.596%	
3) 1,2-DCA-D4(S)	5.98	65	85552	27.99	ppb	0.17
Spiked Amount	25.000		Recovery	=	111.948%	
5) Toluene-D8(S)	8.08	98	397906	24.21	ppb	0.13
Spiked Amount	25.000		Recovery	=	96.852%	
6) 4-Bromofluorobenzene(S)	10.70	95	162293	25.31	ppb	0.11
Spiked Amount	25.000		Recovery	=	101.252%	

Target Compounds

Qvalue

Quantitation Report


Data File : M:\MAX\DATA\211015\1026M31.D
Acq On : 26 Oct 21 23:20
Sample : 211026B BLK
Misc : IS&S 8/4/21

Vial: 31
Operator: LP,DG,CH
Inst : Max
Multiplr: 1.00

Quant Time: Nov 30 13:11 2021

Quant Results File: MGAS0825.RES

Method : M:\MAX\DATA\211015\MGAS0825.M (RTE Integrator)
Title : METHOD 8260B
Last Update : Thu Aug 26 16:19:36 2021
Response via : Initial Calibration

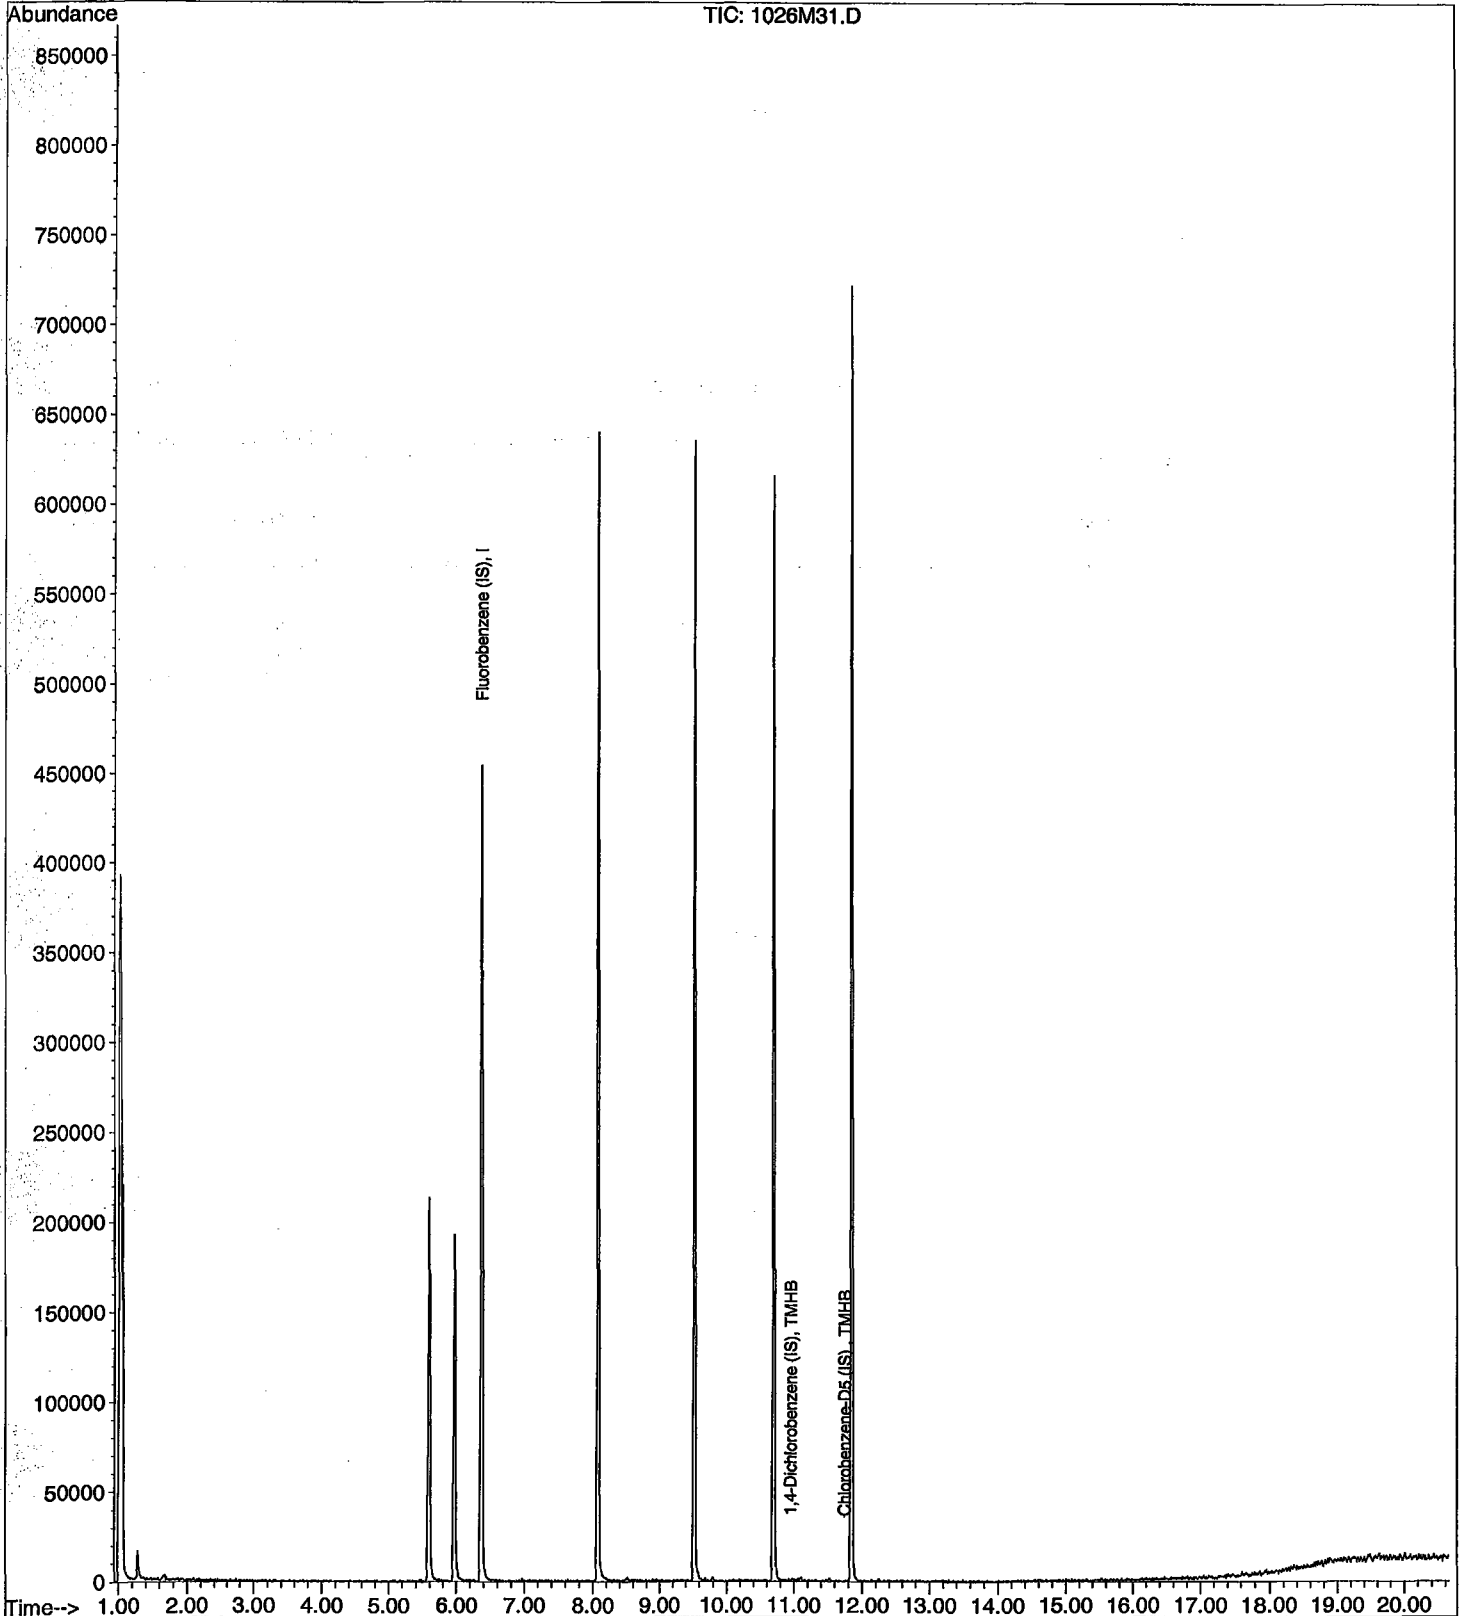

Quantitation Report (QT Reviewed)

Data File : M:\MAX\DATA\211015\1026M29.D
 Acq On : 26 Oct 21 22:23
 Sample : 211026B LCS 300ug/L
 Misc : IS&S 8/4/21

Vial: 29
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 27 9:53 2021

Quant Results File: MGAS0825.RES

Quant Method : M:\MAX\DATA\210922\MGAS0825.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Thu Aug 26 16:19:36 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.37	TIC	439051	25.00	ppb	0.16
3) Chlorobenzene-D5 (IS)	11.75	TIC	1165967m	25.00	ppb	0.00
4) 1,4-Dichlorobenzene (IS)	10.94	TIC	111331m	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Gasoline C6-C10	8.08	TIC	6834012m	324.98	ppb	100

Data File : M:\MAX\DATA\211015\1026M29.D
 Acq On : 26 Oct 21 22:23
 Sample : 211026B LCS 300ug/L
 Misc : IS&S 8/4/21

Vial: 29
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Nov 30 12:58 2021

Quant Results File: M0825SUR.RES

Quant Method : M:\MAX\DATA\210825\M0825SUR.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Thu Aug 26 11:16:48 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.37	96	368670	25.00	ppb	0.16
4) Chlorobenzene-D5 (IS)	9.53	117	341910	25.00	ppb	0.12
7) 1,4-Dichlorobenzene-D (IS)	11.85	152	223205	25.00	ppb	0.10
System Monitoring Compounds						
2) Dibromofluoromethane(S)	5.59	111	121452	27.32	ppb	0.18
Spiked Amount	25.000		Recovery	=	109.264%	
3) 1,2-DCA-D4 (S)	5.98	65	81424	27.87	ppb	0.17
Spiked Amount	25.000		Recovery	=	111.472%	
5) Toluene-D8 (S)	8.08	98	387147	24.15	ppb	0.13
Spiked Amount	25.000		Recovery	=	96.584%	
6) 4-Bromofluorobenzene(S)	10.70	95	158025	25.26	ppb	0.11
Spiked Amount	25.000		Recovery	=	101.048%	

Target Compounds

Qvalue

Quantitation Report


Data File : M:\MAX\DATA\211015\1026M29.D
Acq On : 26 Oct 21 22:23
Sample : 211026B LCS 300ug/L
Misc : IS&S 8/4/21

Vial: 29
Operator: LP,DG,CH
Inst : Max
Multiplr: 1.00

Quant Time: Oct 27 9:53 2021

Quant Results File: MGAS0825.RES

Method : M:\MAX\DATA\211015\MGAS0825.M (RTE Integrator)
Title : METHOD 8260B
Last Update : Thu Aug 26 16:19:36 2021
Response via : Initial Calibration

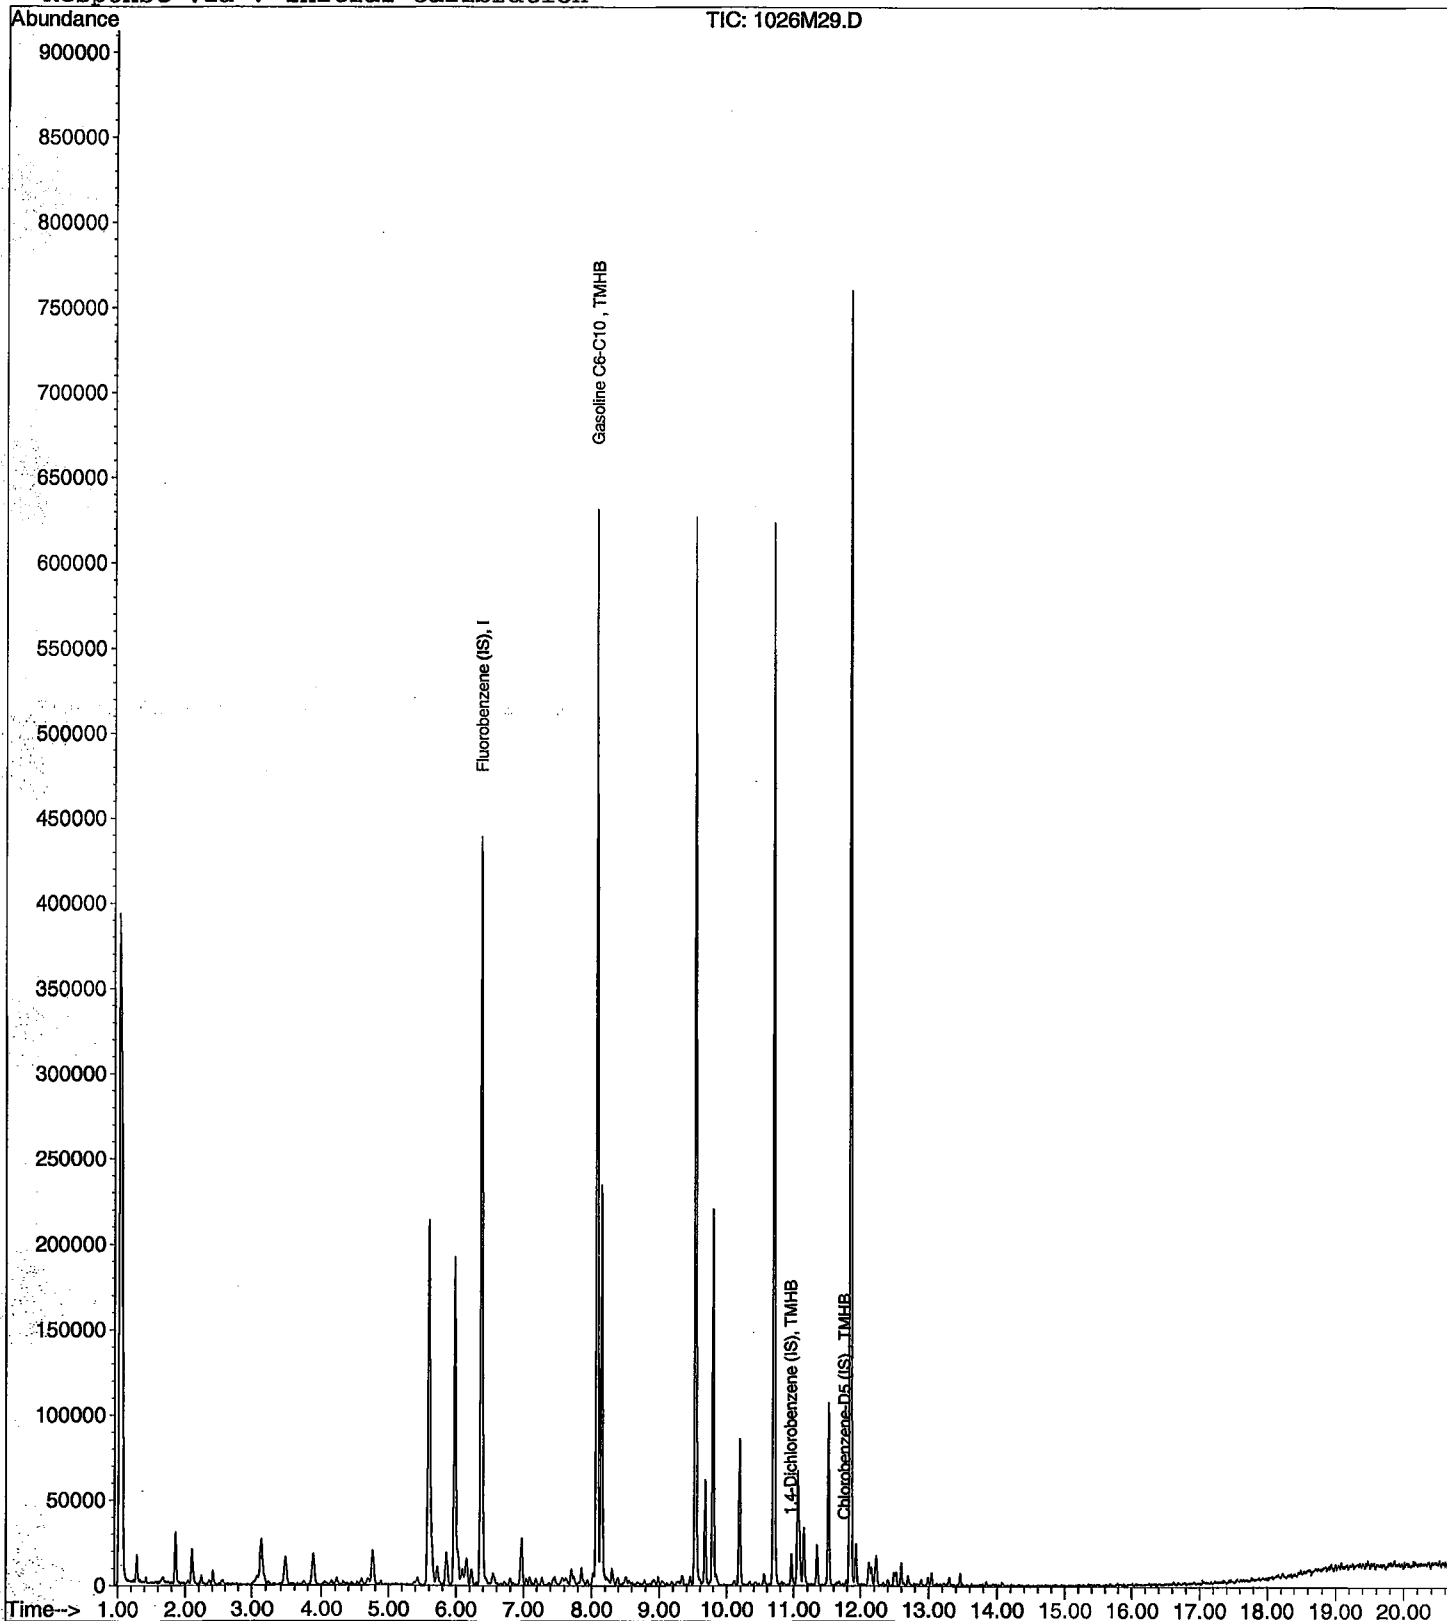

Quantitation Report (QT Reviewed)

Data File : M:\MAX\DATA\211015\1026M30.D
 Acq On : 26 Oct 21 22:51
 Sample : 211026B LCSD 300ug/L
 Misc : IS&S 8/4/21

Vial: 30
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Oct 27 9:55 2021

Quant Results File: MGAS0825.RES

Quant Method : M:\MAX\DATA\210922\MGAS0825.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Thu Aug 26 16:19:36 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.37	TIC	440530	25.00	ppb	0.16
3) Chlorobenzene-D5 (IS)	11.75	TIC	1177830m	25.00	ppb	0.00
4) 1,4-Dichlorobenzene (IS)	10.94	TIC	132726m	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Gasoline C6-C10	8.08	TIC	7068690m	357.30	ppb	100

Data File : M:\MAX\DATA\211015\1026M30.D
 Acq On : 26 Oct 21 22:51
 Sample : 211026B LCSD 300ug/L
 Misc : IS&S 8/4/21

Vial: 30
 Operator: LP,DG,CH
 Inst : Max
 Multiplr: 1.00

Quant Time: Nov 30 12:58 2021

Quant Results File: M0825SUR.RES

Quant Method : M:\MAX\DATA\210825\M0825SUR.M (RTE Integrator)
 Title : METHOD 8260B
 Last Update : Thu Aug 26 11:16:48 2021
 Response via : Initial Calibration
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.37	96	364937	25.00	ppb	0.16
4) Chlorobenzene-D5 (IS)	9.53	117	335196	25.00	ppb	0.11
7) 1,4-Dichlorobenzene-D (IS)	11.85	152	222413	25.00	ppb	0.10
System Monitoring Compounds						
2) Dibromofluoromethane(S)	5.59	111	120694	27.42	ppb	0.18
Spiked Amount	25.000		Recovery	=	109.696%	
3) 1,2-DCA-D4(S)	5.98	65	80816	27.94	ppb	0.17
Spiked Amount	25.000		Recovery	=	111.768%	
5) Toluene-D8(S)	8.08	98	391366	24.90	ppb	0.13
Spiked Amount	25.000		Recovery	=	99.592%	
6) 4-Bromofluorobenzene(S)	10.70	95	156307	25.49	ppb	0.11
Spiked Amount	25.000		Recovery	=	101.952%	

Target Compounds

Qvalue

Quantitation Report


Data File : M:\MAX\DATA\211015\1026M30.D
Acq On : 26 Oct 21 22:51
Sample : 211026B LCSD 300ug/L
Misc : IS&S 8/4/21

Vial: 30
Operator: LP,DG,CH
Inst : Max
Multiplr: 1.00

Quant Time: Oct 27 9:55 2021

Quant Results File: MGAS0825.RES

Method : M:\MAX\DATA\211015\MGAS0825.M (RTE Integrator)
Title : METHOD 8260B
Last Update : Thu Aug 26 16:19:36 2021
Response via : Initial Calibration

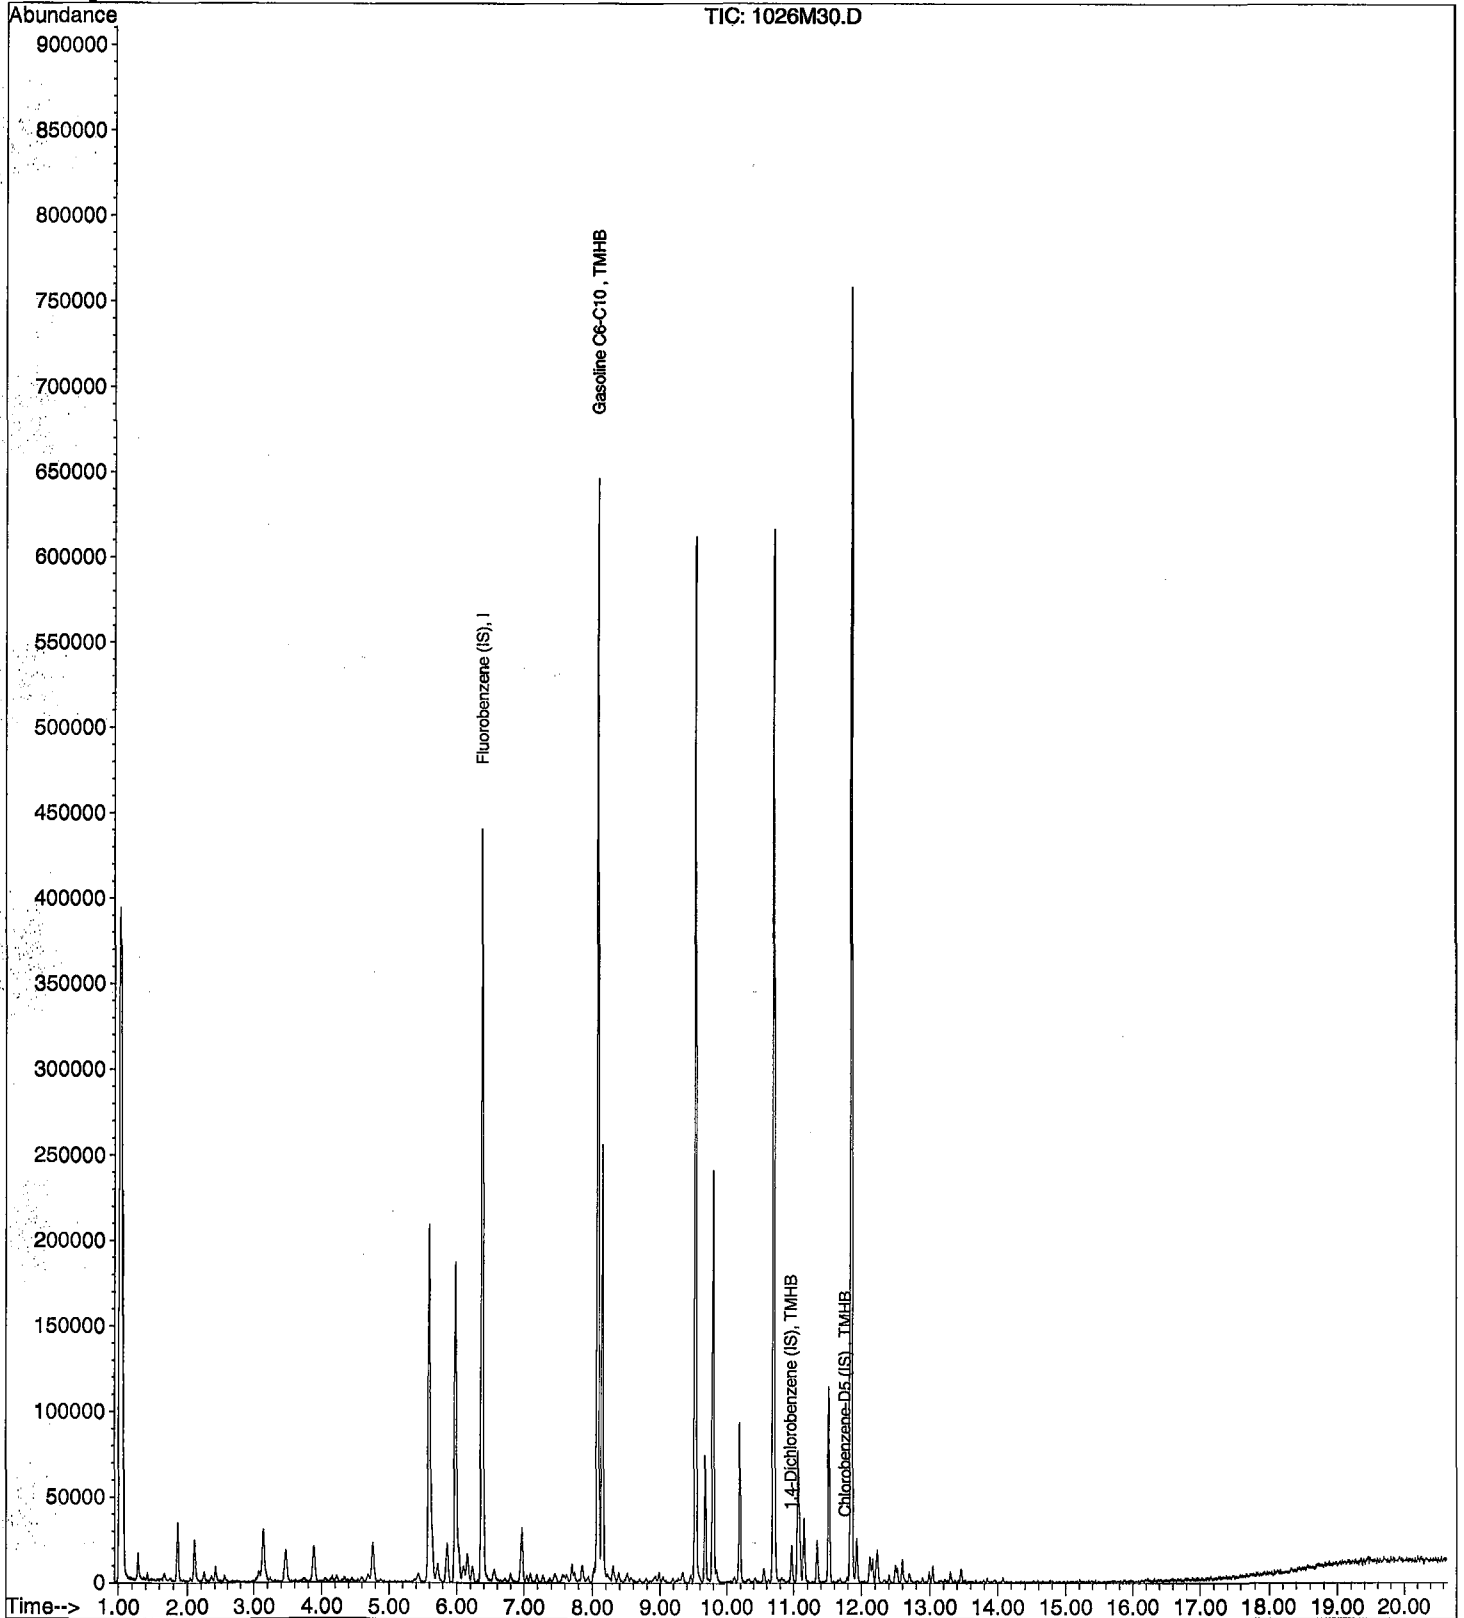

MAX Gas Standard Prep

Gas Primary Working Standard										
Prepared: 6/23/2021						Prepared By (Initials): CH				
Expires: 1/4/2022										
Methanol Lot No.										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	Supplier P/N#	Conc. (ug/mL)	Lot Number - QA Number	Exp. Date (1 yr)	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/mL)
50,000ug/mL Gas STD	Restek	30205	50,000	A0132443	1/4/2022	12/31/2024	80uL	2mL	Methanol	2,000
Gas Second Source (SS) Working Standard										
Prepared: 3/31/2021						Prepared By (Initials): CH				
Expires: 1/31/1930										
Methanol Lot No.										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	Supplier P/N#	Conc. (ug/mL)	Lot Number - QA Number	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/mL)
Gasoline (50,000ppm)	Phenova	ALO-101543	50,000	CL14915-51175	1/4/2022	1/31/1930	80uL	100mL	Methanol	2,000
MAX Gas Calibration Curve										
Prepared: 8/25/2021						Prepared By (Initials): CH				
Expires: 10/24/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA Gasses Standards	Phenova	20ug/L	2,000	Prepared 06/23/21	1/4/2022	N/A	1uL	100mL	P&T Water	20
VOA Gasses Standards	Phenova	50ug/L	2,000	Prepared 06/23/21	1/4/2022	N/A	2.5uL	100mL	P&T Water	50
VOA Gasses Standards	Phenova	100ug/L	2,000	Prepared 06/23/21	1/4/2022	N/A	5uL	100mL	P&T Water	100
VOA Gasses Standards	Phenova	300ug/L	2,000	Prepared 06/23/21	1/4/2022	N/A	15uL	100mL	P&T Water	300
VOA Gasses Standards	Phenova	600ug/L	2,000	Prepared 06/23/21	1/4/2022	N/A	30uL	100mL	P&T Water	600
VOA Gasses Standards	Phenova	800ug/L	2,000	Prepared 06/23/21	1/4/2022	N/A	40uL	100mL	P&T Water	800
VOA Gasses Standards	Phenova	1,000ug/L	2,000	Prepared 06/23/21	1/4/2022	N/A	50uL	100mL	P&T Water	1,000
Zeus Gas Second Source										
Prepared: 8/25/2021						Prepared By (Initials): CH				
Expires: 10/24/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
50,000ug/mL Gas STD	Phenova	SS 300ug/L	2,000	Prepared 03/31/21	1/31/1930	N/A	15uL	100mL	P&T Water	300
MAX Gas Continuing Calibrations/Lab Control Spikes										
Prepared: 8/25/2021						Prepared By (Initials): CH				
Expires: 8/26/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	Supplier P/N#	Conc. (ug/mL)	Lot Number - QA Number	Exp. Date (1 yr)	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/mL)
VOA Gasses Standards	Phenova	300ug/L	2,000	Prepared 06/23/21	1/4/2022	N/A	15uL	100mL	P&T Water	300

MAX 8260 Standard Prep

MAX 8260 Water Calibration Curve										
0.3ug/L						Prepared By (Initials): CH				
Prepared: 8/25/2021										
Expires: 9/8/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 9	Various	0.3ug/L	5	Prepared 08/24/21	10/23/2021	N/A	3uL	50mL	P&T Water	0.3
VOA STD. 1	Absolute		50	Prepared 08/24/21	10/23/2021	N/A	5uL			5
VOA STD. 2	Phenova		100	Prepared 08/24/21	10/23/2021	N/A	2.5uL			5
VOA STD. TBA	Various		250	Prepared 08/24/21	9/8/2021	N/A	2uL			10
0.5ug/L										
Prepared: 8/25/2021										
Expires: 9/8/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 9	Various	0.5ug/L	5	Prepared 08/24/21	10/23/2021	N/A	5uL	50mL	P&T Water	0.5
VOA STD. 1	Absolute		50	Prepared 08/24/21	10/23/2021	N/A	10uL			10
VOA STD. 2	Phenova		100	Prepared 08/24/21	10/23/2021	N/A	5uL			10
VOA STD. TBA	Various		250	Prepared 08/24/21	9/8/2021	N/A	5uL			25
1.0ug/L										
Prepared: 8/25/2021										
Expires: 9/8/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 9	Various	1.0ug/L	5	Prepared 08/24/21	10/23/2021	N/A	10uL	50mL	P&T Water	1
VOA STD. 1	Absolute		50	Prepared 08/24/21	10/23/2021	N/A	20uL			20
VOA STD. 2	Phenova		100	Prepared 08/24/21	10/23/2021	N/A	10uL			20
VOA STD. TBA	Various		250	Prepared 08/24/21	9/8/2021	N/A	10uL			50
2.0ug/L										
Prepared: 8/25/2021										
Expires: 9/8/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 9	Various	2.0ug/L	5	Prepared 08/24/21	10/23/2021	N/A	20uL	50mL	P&T Water	2
VOA STD. 1	Absolute		50	Prepared 08/24/21	10/23/2021	N/A	30uL			30
VOA STD. 2	Phenova		100	Prepared 08/24/21	10/23/2021	N/A	15uL			30
VOA STD. TBA	Various		250	Prepared 08/24/21	9/8/2021	N/A	15uL			75
5ug/L										
Prepared: 8/25/2021										
Expires: 9/8/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	5ug/L	50	Prepared 08/24/21	10/23/2021	N/A	5uL	50mL	P&T Water	5
VOA STD. 8	Phenova		50	Prepared 08/24/21	9/8/2021	N/A	5uL			5
VOA STD. 1	Absolute		50	Prepared 08/24/21	10/23/2021	N/A	40uL			40
VOA STD. 2	Phenova		100	Prepared 08/24/21	10/23/2021	N/A	20uL			20
VOA STD. TBA	Various		250	Prepared 08/24/21	9/8/2021	N/A	20uL			100
10ug/L										
Prepared: 8/25/2021										
Expires: 9/8/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	10ug/L	50	Prepared 08/24/21	10/23/2021	N/A	10uL	50mL	P&T Water	10
VOA STD. 8	Phenova		50	Prepared 08/24/21	9/8/2021	N/A	10uL			10
VOA STD. 1	Absolute		50	Prepared 08/24/21	10/23/2021	N/A	50uL			50
VOA STD. 2	Phenova		100	Prepared 08/24/21	10/23/2021	N/A	25uL			50
VOA STD. TBA	Various		250	Prepared 08/24/21	9/8/2021	N/A	25uL			125

20ug/L										
Prepared: 8/25/2021										
Expires: 9/8/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	20ug/L	50	Prepared 08/24/21	10/23/2021	N/A	20uL	50mL	P&T Water	20
VOA STD. 8	Phenova		50	Prepared 08/24/21	9/8/2021	N/A	20uL			20
VOA STD. 1	Absolute		50	Prepared 08/24/21	10/23/2021	N/A	60uL			60
VOA STD. 2	Phenova		100	Prepared 08/24/21	10/23/2021	N/A	30uL			60
VOA STD. TBA	Various		250	Prepared 08/24/21	9/8/2021	N/A	30uL			150
40ug/L										
Prepared: 8/25/2021										
Expires: 9/8/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	40ug/L	50	Prepared 08/24/21	10/23/2021	N/A	40uL	50mL	P&T Water	40
VOA STD. 8	Phenova		50	Prepared 08/24/21	9/8/2021	N/A	40uL			40
VOA STD. 1	Absolute		50	Prepared 08/24/21	10/23/2021	N/A	80uL			80
VOA STD. 2	Phenova		100	Prepared 08/24/21	10/23/2021	N/A	40uL			80
VOA STD. TBA	Various		250	Prepared 08/24/21	9/8/2021	N/A	35uL			175
100ug/L										
Prepared: 8/25/2021										
Expires: 9/8/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	100ug/L	50	Prepared 08/24/21	10/23/2021	N/A	100uL	50mL	P&T Water	100
VOA STD. 8	Phenova		50	Prepared 08/24/21	9/8/2021	N/A	100uL			100
VOA STD. 1	Absolute		50	Prepared 08/24/21	10/23/2021	N/A	100uL			100
VOA STD. 2	Phenova		100	Prepared 08/24/21	10/23/2021	N/A	50uL			100
VOA STD. TBA	Various		250	Prepared 08/24/21	9/8/2021	N/A	40uL			200
MAX 8260 Water Second Source (SS)										
Prepared: 8/25/2021										
Expires: 9/8/2021										
						Prepared By (Initials): CH				
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 3	Phenova	8260 Water SS	100	Prepared 08/24/21	10/23/2021	N/A	25uL	50mL	P&T Water	50
VOA STD. GASES	Phenova	8260 Water SS	50	Prepared 08/24/21	10/23/2021	N/A	10uL			10
VOA STD. 0	Phenova	8260 Water SS	50	Prepared 08/24/21	10/23/2021	N/A	10uL			10
VOA STD. 2-CEVE	Absolute	8260 Water SS	50	Prepared 08/24/21	8/24/2021	N/A	50uL			50
VOA STD. 6	Various	8260 Water SS	50	Prepared 08/24/21	9/8/2021	N/A	10uL			10
Voa STD. TBA	Various	8260 Water SS	250	Prepared 08/24/21	9/8/2021	N/A	25uL	250		
8260 Water Continuing Calibrations (CCV)/ Lab Control Spikes (LCS)										
Prepared: 8/25/2021										
Expires: 8/26/2021										
						Prepared By (Initials): CH				
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	CCV/ LCS	50	Prepared 08/24/21	10/23/2021	N/A	10uL	50mL	P&T Water	10
VOA STD. 8	Phenova	CCV/ LCS	50	Prepared 08/24/21	9/8/2021	N/A	10uL			10
VOA STD. 1	Absolute	CCV/ LCS	50	Prepared 08/24/21	10/23/2021	N/A	50uL			50
VOA STD. 2	Phenova	CCV/ LCS	100	Prepared 08/24/21	10/23/2021	N/A	25uL			50
VOA STD. TBA	Various	CCV/ LCS	250	Prepared 08/24/21	9/8/2021	N/A	25uL			250

Injection Log


Directory: M:\MAX\DATA\210825\

Line	Vial	FileName	Multiplier	SampleName	Misc Info	Injected
1	2	0825M12.D	1	0.3ug/L VOC STD 8/25/21	IS&S 6/4/21	25 Aug 21 15:15
2	3	0825M13.D	1	0.5ug/L VOC STD 8/25/21	IS&S 6/4/21	25 Aug 21 15:43
3	4	0825M14.D	1	1ug/L VOC STD 8/25/21	IS&S 6/4/21	25 Aug 21 16:11
4	5	0825M15.D	1	2ug/L VOC STD 8/25/21	IS&S 6/4/21	25 Aug 21 16:39
5	6	0825M16.D	1	5ug/L VOC STD 8/25/21	IS&S 6/4/21	25 Aug 21 17:07
6	7	0825M17.D	1	10ug/L VOC STD 8/25/21	IS&S 6/4/21	25 Aug 21 17:35
7	8	0825M18.D	1	20ug/L VOC STD 8/25/21	IS&S 6/4/21	25 Aug 21 18:03
8	9	0825M19.D	1	40ug/L VOC STD 8/25/21	IS&S 6/4/21	25 Aug 21 18:31
9	10	0825M20.D	1	100ug/L VOC STD 8/25/21	IS&S 6/4/21	25 Aug 21 18:59
10	13	0825M23.D	1	20ug/L GAS STD 8/25/21	IS&S 6/4/21	25 Aug 21 20:23
11	14	0825M24.D	1	50ug/L GAS STD 8/25/21	IS&S 6/4/21	25 Aug 21 20:51
12	15	0825M25.D	1	100ug/L GAS STD 8/25/21	IS&S 6/4/21	25 Aug 21 21:19
13	16	0825M26.D	1	300ug/L GAS STD 8/25/21	IS&S 6/4/21	25 Aug 21 21:47
14	17	0825M27.D	1	600ug/L GAS STD 8/25/21	IS&S 6/4/21	25 Aug 21 22:14
15	18	0825M28.D	1	800ug/L GAS STD 8/25/21	IS&S 6/4/21	25 Aug 21 22:42
16	19	0825M29.D	1	1000ug/L GAS STD 8/25/21	IS&S 6/4/21	25 Aug 21 23:10
17	21	0825M31.D	1	(SS) 300ug/L GAS STD 8/25/21	IS&S 6/4/21	26 Aug 21 00:06
1	28	1026M28.D	1	211026B CCV 300ug/L	IS&S 8/4/21	26 Oct 21 21:55
2	29	1026M29.D	1	211026B LCS 300ug/L	IS&S 8/4/21	26 Oct 21 22:23
3	30	1026M30.D	1	211026B LCSD 300ug/L	IS&S 8/4/21	26 Oct 21 22:51
4	31	1026M31.D	1	211026B BLK	IS&S 8/4/21	26 Oct 21 23:20
5	35	1026M35.D	1	BA43836W01	IS&S 8/4/21	27 Oct 21 1:13
6	36	1026M36.D	1	BA43837W01	IS&S 8/4/21	27 Oct 21 1:41
7	46	1026M46.D	1	Ending CCV 300ug/L 10/26/21	IS&S 8/4/21	27 Oct 21 6:23

INORGANIC ANALYSIS
Calibration and Raw Data

Method: WetChem	TOTAL ORGANIC CARBON	Instrument: Tic Toc
Analyte: TOC	Units mg/L	
Analyst: EA	QCG: 211027A	
	Final Volume: 40mL	

Date	Time	Appl ID	[TOC]	Raw	% Recovery
10/25/2021	19:20	QC blank	0.00	4558	
10/25/2021	19:56	Ical 1	0.50	9475	
10/25/2021	20:28	Ical 2	2.00	29763	
10/25/2021	21:02	Ical 3	5.00	69278	
10/25/2021	21:35	Ical 4	10.00	139847	
10/25/2021	22:08	Ical 5	20.00	273227	
10/25/2021	10:03	ICB	0.08	2197	
10/25/2021	10:39	ICV	10.40	144915	105.5%

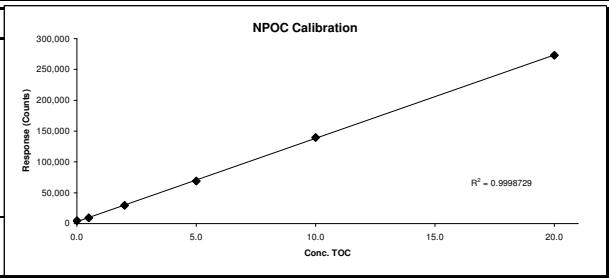

Date	Time	Appl ID	DF	Raw Result	SubSample Amount	Filter Blank Subtract	Calc Conc	Result	Range (mg/L)	QC True	% Recovery
2021-10-27	04:14 PM	QCB	1	2894	40mL	0.000	0	0.00	0.00		
2021-10-27	09:24 PM	211027A CCV	1	71753	40mL	0.000	5.102	5.10	0.04	5.00	102.0%
2021-10-27	10:10 PM	211027A CCB	1	2333	40mL	0.000	0	0.00	0.00		
2021-10-27	10:55 PM	211027A LCS	1	72028	40mL	0.000	5.123	5.12	0.00	5.00	102.5%
2021-10-27	11:41 PM	211027A LCSD	1	71352	40mL	0.000	5.073	5.07	0.01	5.00	101.5%
2021-10-28	12:27 AM	BA43832W05	1	5605	40mL	0.000	0.232	0.23	0.05		
2021-10-28	01:10 AM	BA44243W01	1	127193	40mL	0.000	9.241	9.24	0.15		
2021-10-28	01:53 AM	BA44244W02	1	13898	40mL	0.000	0.846	0.85	0.08		
2021-10-28	02:35 AM	BA43839W02	1	8474	40mL	0.000	0.444	0.44	0.00		
2021-10-28	03:17 AM	BA43840W01	1	4994	40mL	0.000	0.186	0.19	0.03		
2021-10-28	03:58 AM	BA43837W05	1	4837	40mL	0.000	0.175	0.18	0.02		
2021-10-28	04:40 AM	BA43157W02	1	7965	40mL	0.000	0.406	0.41	0.05		
2021-10-28	05:21 AM	BA43156W01	1	4741	40mL	0.000	0.167	0.17	0.04		
2021-10-28	06:03 AM	BA43555W02	1	4787	40mL	0.000	0.171	0.17	0.01		
2021-10-28	06:45 AM	CCV	1	72640	40mL	0.000	5.168	5.17	0.07	5.00	103.4%
2021-10-28	07:31 AM	211027B CCB	1	2430	40mL	0.000	0	0.00	0.00		
2021-10-28	08:16 AM	BA43151W06	1	219427	40mL	0.000	16.075	16.08	0.06		
2021-10-28	08:59 AM	BA43158W02	1	6431	40mL	0.000	0.293	0.29	0.04		
2021-10-28	09:41 AM	BA44220W05 5310C	1	23329	40mL	0.000	1.545	1.55	0.00		
2021-10-28	10:24 AM	BA44221W05 5310C	1	18979	40mL	0.000	1.222	1.22	0.02		
2021-10-28	11:06 AM	BA44044W01	1	4697	40mL	0.000	0.164	0.16	0.02		
2021-10-28	11:49 AM	BA44045W02	1	11307	40mL	0.000	0.654	0.65	0.01		
2021-10-28	12:32 PM	BA44046W02	1	6046	40mL	0.000	0.264	0.26	0.03		
2021-10-28	01:14 PM	BA44048W05	1	6209	40mL	0.000	0.276	0.28	0.02		
2021-10-28	01:56 PM	BA44050W06	1	65464	40mL	0.000	4.667	4.67	0.27		
2021-10-28	02:40 PM	BA44052W05	1	38074	40mL	0.000	2.638	2.64	0.12		
2021-10-28	03:24 PM	CCV	1	68803	40mL	0.000	4.884	4.88	0.31	5.00	97.7%
2021-10-28	04:10 PM	CCB	1	2389	40mL	0.000	0	0.00	0.00		

Name of Final Standard **TOC Calibration Curve**
 Prep Date 10/25/2021
 Exp Date 10/25/2022

Prep'd By (Initials) KS

Initial Standard Information						Final Standard Information			
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc.(range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
Total Organic Carbon (TOC) Standard Cal 1	Agilent	IQC-106-5	1000 mg/L	0006588597-51848	3/31/2023	20 uL	40 mL	DI Water	0.5 ppm
Total Organic Carbon (TOC) Standard Cal 2	Agilent	IQC-106-5	1000 mg/L	0006588597-51848	3/31/2023	80 uL	40 mL	DI Water	2 ppm
Total Organic Carbon (TOC) Standard Cal 3	Agilent	IQC-106-5	1000 mg/L	0006588597-51848	3/31/2023	200 uL	40 mL	DI Water	5 ppm
Total Organic Carbon (TOC) Standard Cal 4	Agilent	IQC-106-5	1000 mg/L	0006588597-51848	3/31/2023	400 uL	40 mL	DI Water	10 ppm
Total Organic Carbon (TOC) Standard Cal 5	Agilent	IQC-106-5	1000 mg/L	0006588597-51848	3/31/2023	800 uL	40 mL	DI Water	20 ppm

Name of Final Standard **ICV (TOC)**
 Prep Date 10/25/2021
 Exp Date 10/25/2022

Prep'd By (Initials) KS

Initial Standard Information						Final Standard Information			
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc.(range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
1000 PPM ICV TOC Intermediate	APPL Inc.	IQC-106-5	1000 mg/L	0006465171-49409	6/30/2021	400 uL	40mL	DI Water	10 ppm

ICV recertified against the non-expired calibration

Name of Final Standard **CCV (TOC)**
 Prep Date See Data
 Exp Date 1 year

Prep'd By (Initials) EA

Initial Standard Information						Final Standard Information			
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc.(range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
Total Organic Carbon (TOC) Standard	Agilent	IQC-1 06-5	1000 mg/L	0006588597-51848	3/31/2023	200 uL	40 mL	DI Water	5 ppm

Name of Final Standard **TOC LCS/LCSD**
 Prep Date See Data
 Exp Date 1 year

Prep'd By (Initials) EA

Initial Standard Information						Final Standard Information			
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc.(range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
Total Organic Carbon (TOC) Standard	Agilent	IQC-106-5	1000 mg/L	0006588597-51848	3/31/2023	200 uL	40 mL	DI Water	5 ppm

Name of Final Standard **TOC MS/MSD**
 Prep Date See Data
 Exp Date 1 year

Prep'd By (Initials) EA

Initial Standard Information						Final Standard Information			
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc.(range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
Total Organic Carbon (TOC) Standard	Agilent	IQC-106-5	1000 mg/L	0006588597-51848	3/31/2023	200 uL	40 mL	sample	5 ppm