



908 North Temperance Ave. ▽ Clovis, CA 93611 ▽ Phone 559-275-2175 ▽ Fax 559-275-4422

Certification Number: CA1312  
NELAP Certification number: CA00046  
DoD-ELAP Certificate number: 4064.01

## Data Validatable Report

January 17, 2022

AECOM  
1001 Bishop Street, Suite 1600  
Honolulu, Hawaii 96813

Attn: Alethea Ramos

Title: Report of Data: Case 98212

Project: 60571032 CV18F0126 Red Hill Fuel Storage, HI

Contract #: Prime contract # for DoD: NAVY CLEAN N62742-17-F-1800, CV18F0126  
Subcontract: 18S-22209-HI27

Dear Ms. Ramos:

Four water samples were received November 12, 2021. Sample ER1915 (BA46117) was canceled per client request. Written results for the requested analyses are being provided on this January 17, 2022.

Results in this report apply to the samples analyzed in accordance with the chain of custody document. This analytical report must be reproduced in its entirety.

If you have any questions or require further information, please contact your APPL Project Manager, Libby Cheeseborough, libby@applinc.com, at your convenience. Thank you for choosing APPL, Inc.

I certify that this data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. These test results meet all requirements of NELAC and DoD QSM. Release of the hard copy has been authorized by the Laboratory Manager or his designee, as verified by the following signature.

Loren Portwood, Laboratory Director  
APPL, Inc.

LP/lac  
Enclosure  
cc: File

Data Validation Package  
for  
60571032 CV18F0126 Red Hill Fuel Storage  
APPL SDG 98212  
TABLE OF CONTENTS

LABORATORY NAME: APPL, Inc.

Case Narrative	<u>3</u>
Sample Management Records	<u>7</u>
Sample Results	<u>14</u>
QC Forms	<u>30</u>
Method 8015B Calibration Data	<u>90</u>
Method 8015B Raw Data	<u>116</u>
Method 8015B Silica Gel Calibration Data	<u>134</u>
Method 8015B Silica Gel Raw Data	<u>179</u>
Method 8015B Blank Calibration Data	<u>200</u>
Method 8015B Blank Raw Data	<u>229</u>
Method 8270D SIM Calibration Data	<u>246</u>
Method 8270D SIM Raw Data	<u>273</u>
Method 8260B Calibration Data	<u>300</u>
Method 8260B Raw Data	<u>427</u>
Method 8260B GRO Calibration Data	<u>458</u>
Method 8260B GRO Raw Data	<u>551</u>
Inorganic Analyses and Calibration Raw Data	<u>589</u>

# **CASE NARRATIVE**

# Case Narrative

ARF: 98212

Project: 60571032 CV18F0126 Red Hill Fuel Storage. HI

## Sample Receipt Information:

Four water samples were received November 12, 2021 at  $-0.9^{\circ}\text{C}$  and  $1.0^{\circ}\text{C}$ . The sample group was assigned Analytical Request Form (ARF) number 98212. Sample ER1915 (BA46117) was canceled per client request.

## Sample Preparation and Analysis Information:

For the EPA 8015B analysis, the samples were extracted according to EPA method 3520C. The sample extracts were silica gel cleaned according to APPL's SOP CLN004 and analyzed.

For the EPA 8015B analysis, pre-extraction sample blanks were extracted according to EPA method 3520C before the method QC and field samples. The sample blanks are included in this report.

For the EPA 8270D SIM analysis, the samples were extracted according to EPA method 3520C.

For the EPA 8260B analysis, the samples were purged according to EPA method 5030B.

For the EPA 9060A analysis, the samples were prepared according to the methods.

Only the portion of the injection log relative to these samples is included. A full sequence log is available upon request. Measurement uncertainty can be reported upon request.

## Analytical Exceptions, Deviations and Abnormalities.

**EPA 8015B:** In the 211116A method blank, Oil was detected above one-half the LOQ. Corrective action: Five samples were B-flagged for Oil. The 211116A-LCS recovers Oil above the upper control limit.

**EPA 8015B SGC:** In the 211116A1 method blank, Oil was detected above one-half the LOQ. The 211116A1-LCS recovers Oil above the upper control limit. Corrective action: None. There were no Oil detections in the samples.

**EPA 8015B Blank:** One sample recovers one surrogate below the lower control limit.

qryCOC\_APPLCaseNarrativeReport

<b>SDG</b>	<b>Received</b>	<b>Client ID</b>	<b>APPL ID</b>	<b>Collected DateTime</b>	<b>Matrix</b>	<b>Method</b>	<b>Method Description</b>
98212	11/12/2021	ERH1906	BA46114	11/10/2021 11:20:00 AM	WATER	EPA 8260B	EPA 8260B BTEX WATER
98212	11/12/2021	ERH1906	BA46114	11/10/2021 11:20:00 AM	WATER	EPA 8260B	EPA 8260B GRO WATER
98212	11/12/2021	ERH1907	BA46115	11/10/2021 11:35:00 AM	WATER	EPA 8260B	EPA 8260B BTEX WATER
98212	11/12/2021	ERH1907	BA46115	11/10/2021 11:35:00 AM	WATER	EPA 8015B-eHL	EPA 8015B TPH WATER L-L SGC
98212	11/12/2021	ERH1907	BA46115	11/10/2021 11:35:00 AM	WATER	EPA 8015B-eHL	EPA 8015B TPH LIQ-LIQ
98212	11/12/2021	ERH1907	BA46115	11/10/2021 11:35:00 AM	WATER	EPA 8260B	EPA 8260B GRO WATER
98212	11/12/2021	ERH1907	BA46115	11/10/2021 11:35:00 AM	WATER	8270D-SIM	EPA 8270D SIM LIQ-LIQ
98212	11/12/2021	ERH1907	BA46115	11/10/2021 11:35:00 AM	WATER	SW846 9060A	9060A TOC
98212	11/12/2021	ERH1909	BA46116	11/10/2021 11:35:00 AM	WATER	EPA 8260B	EPA 8260B BTEX WATER
98212	11/12/2021	ERH1909	BA46116	11/10/2021 11:35:00 AM	WATER	EPA 8015B-eHL	EPA 8015B TPH WATER L-L SGC
98212	11/12/2021	ERH1909	BA46116	11/10/2021 11:35:00 AM	WATER	EPA 8015B-eHL	EPA 8015B TPH LIQ-LIQ
98212	11/12/2021	ERH1909	BA46116	11/10/2021 11:35:00 AM	WATER	EPA 8260B	EPA 8260B GRO WATER
98212	11/12/2021	ERH1909	BA46116	11/10/2021 11:35:00 AM	WATER	8270D-SIM	EPA 8270D SIM LIQ-LIQ
98212	11/12/2021	ERH1907 BLANK	BA46118	11/10/2021 11:35:00 AM	WATER	EPA 8015B-eHL	EPA 8015B TPH LIQ-LIQ
98212	11/12/2021	ERH1909 BLANK	BA46119	11/10/2021 11:35:00 AM	WATER	EPA 8015B-eHL	EPA 8015B TPH LIQ-LIQ

## Abbreviations and Flags


FLAG	DESCRIPTION
#	Recovery or RPD outside control limits
*	Recovery or RPD outside control limits
B	Analyte detected in associated method blank
C1	Reason for correction: wrote incorrect response
C2	Reason for correction: calculated incorrectly
C3	Reason for correction: needs to be rechecked
C4	Reason for correction: data not usable
DO	Diluted out
E	Exceeds linear range
F	Estimated value
G1	Includes a wide range of hydrocarbons which does not match our gasoline standard
G10	Includes a match to hydrocarbon profiles within the range of mineral spirits
G11	Includes a match to hydrocarbon profiles within the range of JP-4
G12	Pattern does not match the gasoline standard; the carbon range for this sample is consistent with JP8
G13	Closely resembles the hydrocarbon profile of aviation gasoline
G14	Analyte concentration may be biased due to carry over
G2	Closely resembles the boiling point hydrocarbon profile consistent with weathered gasoline
G3	Includes higher boiling hydrocarbons
G4	Includes dominant peak(s) not indicative of petroleum hydrocarbons
G5	Is mainly dominant peak(s) not indicative of petroleum hydrocarbons
G6	Contains recognizable contaminant peak(s) which has been removed from quantitation
G7	Is mainly a match to hydrocarbons within the range of gasoline
G8	Closely resembles the boiling point hydrocarbon profile consistent with weathered gasoline
G9	Includes hydrocarbons within the range of kerosene
J	Estimated value
M	Matrix effect
MI1	Manual integration: integration does not follow baseline
MI2	Manual integration: non-target peak interference
MI3	Manual integration: to split a peak that was integrated as one peak by the computer
MI4	Manual integration: to integrate a split peak
MI5	Manual integration: the whole peak or part of the peak was not integrated
MI6	Manual integration: computer integrated wrong peak
MI7	Manual integration: other - explain
MDL	Method detection limit
ND	Not detected
NT	Non-target
Q	Acceptance criteria not met
T1 I	Includes wide range of hydrocarbons not indicative of diesel
T1 M	Is mainly wide range of hydrocarbons not necessarily indicative of diesel
T2 I	Includes lower boiling hydrocarbons, i.e. mineral spirits, kerosene, stoddard solvent, white gas
T2 M	Is mainly lower boiling hydrocarbons, i.e. mineral spirits, kerosene, stoddard solvent, white gas
T3 I	Includes higher boiling hydrocarbons, i.e. asphaltene, waster oil, motor oil, or weathered diesel fuel
T3 M	Is mainly higher boiling hydrocarbons, i.e. asphaltene, waster oil, motor oil, or weathered diesel fuel
T4 I	Includes dominant peak(s) not indicative of hydrocarbons
T4 M	Is mainly dominant peak(s) not indicative of hydrocarbons
T5	Contains recognizable contaminant peak(s) which has been removed from quantitation
T6	Is mainly a match to hydrocarbons within range of diesel fuel
T7	Closely resembles the boiling point hydrocarbon profile consistent with diesel fuel
T8	Includes a match to hydrocarbon profiles within range of diesel and kerosene fuel
T9 I	Includes non-diesel hydrocarbons within boiling point range of diesel fuel
T9 M	Is mainly non-diesel hydrocarbons within boiling point range of diesel fuel.
Y	Percent difference between primary and confirmation column > 40%

**SAMPLE RECORDS MANAGEMENT  
CHAIN OF CUSTODY,  
ARF, CRF, AND  
CLIENT COMMUNICATION**

# APPL - Analysis Request Form

98212

Client: AECOM  
 Address: 1001 Bishop Street, Suite 1600  
Honolulu, HI 96813  
 Attn: Alethea Ramos  
 Phone: 808-954-4536 Fax: 808-523-8950  
 Job: 60571032 CV18F0126 Red Hill Fuel Storage  
 PO #: 18S-22209-HI27 PO# 102604  
 Chain of Custody (Y/N): Y # 53189  
 RAD Screen (Y/N): Y pH (Y/N): Y  
 Turn Around Type: 1 WEEK

Received by: MSA   
 Date Received: 11/12/21 Time: 11:30  
 Delivered by: FEDEX  
 Shuttle Custody Seals (Y/N): Y Time Zone: -10  
 Chest Temp(s): -0.9,1.0°C  
 Color: VFRG/Receiving  
 Samples Chilled until Placed in Refrig/Freezer: Y  
 Project Manager: Libby Cheesebor  
 QC Report Type: DVP4DOD/EQUIS/HI  
 Due Date: 11/19/21

Comments:

*PM: login and F1s to Margie.Pascua@aecom.com & alethea.ramos@aecom.com*  
*AN: INCLUDE STANDARD PREP SHEETS!!!!!!*  
*AN: 7 day TAT for Form 1s; 21 day TAT for PKG STYLE 1; DOD v5.1; DOD Forms: LOD database*  
*Report MS/MSD/DUPs when AECOM sample used*  
*8270 SIM: 1-methylnaphthalene, 2-methylnaphthalene & naphthalene only.*  
*TPH-D/O both with and w/o SGC, reverse surrog for SGC; analyze SGC; DO NOT Q-DELETE.*  
*FR: email ftp info to Margie, alethea.ramos@aecom.com, Stella, trommelfanger@lab-data.com & jcanlas@la*  
*EDD: AECOM EQUIS EDD 2.5.3 to alethea.ramos@, Margie.Pascua@aecom.com, jecklund@lab-data.com*  
*EDD: AECOM EDD to alethea.ramos@, Margie.Pascua@aecom.com, jecklund@lab-data.com*




Sample Distribution:

**GC: 3-\$DOC53SGCW5LIQ, 3-\$DOC53W5LIQ, 3-\$SIM53LIQ51, 3-\$RHBLKETBLK**  
**Extractions: 3- LIQ003, 6- LIQ005, 3- LIQ005SGC**  
**VOA: 4-\$86BTOTXDOD5W, 4-\$GASBL, 4-\$GRO86BW**  
**Wetlab: 2-\$TOCW53**

Charges:

Invoice To:

**ACCOUNTS PAYABLE**  
**1001 Bishop Street, Ste 1600**  
**USAPImaging@aecom.com**  
**mary.basano@aecom.com**

Client ID	APPL ID	Sampled	Analyses Requested
1. ERH1906	LCSD BA46114W 	11/10/21 11:20	\$86BTOTXDOD5W, \$GASBL, \$GRO86BW -- See Comments
2. ERH1907	LCSD BA46115W 	11/10/21 11:35	\$86BTOTXDOD5W, \$DOC53SGCW5LIQ, \$DOC53W5LIQ, \$GASBL, \$GRO86BW, \$SIM53LIQ51, \$TOCW53 -- See Comments
3. ERH1909	LCSD BA46116W 	11/10/21 11:35	\$86BTOTXDOD5W, \$DOC53SGCW5LIQ, \$DOC53W5LIQ, \$GASBL, \$GRO86BW, \$SIM53LIQ51 -- See Comments



# APPL - Analysis Request Form

98212

4. ERH1915	LCSD	BA46117W	11/10/21	12:50	\$86BTOTXDOD5W, \$DOC53SGCW5LIQ, \$DOC53W5LIQ, \$GASBL, \$GRO86BW, \$SIM53LIQ51, \$TOCW53 -- EXTRACT & HOLD;See Comments
5. ERH1907 BLANK	LCSD	BA46118W	11/10/21	11:35	\$RHBLKETBLK -- See Comments
6. ERH1909 BLANK	LCSD	BA46119W	11/10/21	11:35	\$RHBLKETBLK -- See Comments
7. ERH1915 BLANK	LCSD	BA46120W	11/10/21	12:50	\$RHBLKETBLK -- See Comments


# APPL Sample Receipt Form

ARF# 98212

Sample	Container Type	Count	p
BA46114	13 VOAs - HCL	4	NA
BA46115	13 VOAs - HCL	4	NA
	17 Amber Liter	2	NA
	32 Clear VOA - H2SO4	2	NA
	39 Amber Liter, HCL prsvd	2	1.3
BA46116	13 VOAs - HCL	4	NA
	17 Amber Liter	2	NA
	39 Amber Liter, HCL prsvd	2	1.3
BA46117	17 Amber Liter	2	NA
	32 Clear VOA - H2SO4	2	NA
	39 Amber Liter, HCL prsvd	2	1.6
BA46118	39 Amber Liter, HCL prsvd	1	NA
BA46119	39 Amber Liter, HCL prsvd	1	NA
BA46120	39 Amber Liter, HCL prsvd	1	NA

Sample    Container Type                    Count    p





APPL, Inc.  
908 N Temperance Ave  
Clovis, CA 93611  
www.applinc.com

CHAIN OF CUSTODY RECORD

Phone: (559) 275-2175  
Fax: (559) 275-4422  
coc@applinc.com C.O.C. 53113 NOI

2/2

Report to: PLEASE PRINT

Company Name: AECOM Phone: (508) 521-3051

Address: 1001 Bishop St, Suite 1600 Fax: 01-18FUR126/

Attn: Alicia Ramos 00571032

Email: Alicia.Ramos@aecom.com

Invoice to: PLEASE PRINT

Company Name: \_\_\_\_\_ Phone: \_\_\_\_\_

Address: \_\_\_\_\_ Fax: \_\_\_\_\_

Attn: Accounts Payable

Email: USAPImaging@aecom.com

Project Name/Number	Sampler (Print)	Date Collected	Time Collected	Time Zone	Matrix			Analysis Requested/Method Number					Date Shipped: <u>11/11/21</u>	Carrier: <u>FedEx</u>	Waybill No.:	Comments: <u>Note: Log NOI in separate SDG from other COC's</u>	
					Aq	Sed	Soil	TR-8-8260C	TR-9-8015C	TR-10-8015C	TR-11-8015C	TR-12-8015C					TR-13-8015C
<u>00571032.02.20.01</u>	<u>DM, NL</u>	<u>Turnham Ave for DM, NL</u>															
<u>102604</u>																	
<u>11-1915</u>	<u>PHSE Post-chlorination</u>	<u>11/10/21</u>	<u>12:50</u>	<u>HST</u>	<u>4</u>	<u>X</u>					<u>X</u>	<u>X</u>				<u>TPH-d/s and PAHs used</u>	<u>liquid-liquid extraction; *Naphthalene</u>
<u>1051</u>																	<u>1-methylnaphthalene</u>
																	<u>2-methylnaphthalene</u>
																	<u>EK-1915 hold until further notice</u>

Shuttle Temperature: \_\_\_\_\_

Turnaround Requested: Check one  
 Standard 2-3 wk  One week  3 days  24/48 Hrs.  Other: \_\_\_\_\_

Relinquished by sampler: \_\_\_\_\_ Received by: \_\_\_\_\_ Date: \_\_\_\_\_

Relinquished by: \_\_\_\_\_ Received by: \_\_\_\_\_ Date: \_\_\_\_\_

Relinquished by: \_\_\_\_\_ Received by: \_\_\_\_\_ Date: \_\_\_\_\_

Relinquished by: \_\_\_\_\_ Received by: \_\_\_\_\_ Date: \_\_\_\_\_

Sample Disposal:  
 Return to client  Disposal by Lab (30-day retention)

White: Return to client with report  
 Yellow: Laboratory Copy  
 See reverse side for Container Preservative and Sampling Information

Received at lab by: Melody Horton  
 Date: 11-12-21 Time: 11:30

COOLER RECEIPT FORM

ARF: 98212

- 1) Project: 60571032 CV18F0126 Red Hill Fuel Storage Date Received: 11/12/2021
- 2) Coolers: Number of Coolers: 2
- 3) YES Were custody seals present and intact?  
How many? 4 Name/Date on seal? SEE BELOW
- 4) YES Was there a shipping slip? Carrier name: FEDEX
- 5) Type of packing in cooler:  bubble wrap  popcorn  foam  plastic bags  other  
 wet ice  dry ice  no ice  gel ice
- 6) YES Were cooler temperatures acceptable?
- 7) Serial number of calibrated thermometer used: R3 CF: -1.9°C; IRB CF: +1.1°C
- 8) Cooler temp(s): In °C. Thermometer Temp / Corrected Temp  
1: 1.0/-0.9° 2: -0.1/1.0° 3: \_\_\_\_\_ 4: \_\_\_\_\_ 5: \_\_\_\_\_ 6: \_\_\_\_\_  
7: \_\_\_\_\_ 8: \_\_\_\_\_ 9: \_\_\_\_\_ 10: \_\_\_\_\_ 11: \_\_\_\_\_ 12: \_\_\_\_\_

Chain of custody:

- 9) YES Was a chain of custody received?
- 10) YES Were the custody papers complete/signed in the appropriate places?

Sample Labels:

- 11) YES Were all sample labels complete (sample ID, date/time of sampling, etc.)?
- 12) YES Did all container labels agree with custody papers?

Sample Containers:

- 13) YES Were all containers sealed in separate bags?
- 14) YES Did all containers arrive in good condition:(unbroken, no leakage, no cracked/broken lids)?
- 15) ~~YES~~ NO YES Were correct containers and preservatives used for the tests indicated?
- 16) YES Was a sufficient amount of sample sent for tests indicated?
- 17) NO Were bubbles present in volatile samples?  
If yes, the following were received with air bubbles:  
Larger than a pea: \_\_\_\_\_  
Smaller than a pea: \_\_\_\_\_

Preservation Hold time:

- 18) YES Was a sufficient amount of holding time remaining to analyze the samples?
- 19) YES Was the pH taken of all non-VOA preserved samples and written on the sample container?
- 20) YES Was the pH of acid preserved non-VOA samples < 2?
- 21) NA Was the pH of the "basic" preserved samples for Cyanide > 12, Sulfide >9, Hexchrom >9?
- 22) NO Were unpreserved VOA Vials received for VOA Dept analysis?
- 23) NA If "yes", are the unpreserved VOA vials noted in the ADD TEST FIELD on the ARF?  
pH strip lot number: HC029115  
Lab notified if pH was not adequate: \_\_\_\_\_

Notes/Deficiencies:

For sample ERH1915, 2 H2SO4 vials were found in the cooler; labeled correctly; but on the COC does not have analysis marked for TOC 9060.

CUSTODY SEAL

APPL, Inc. (559) 275-2175

Initials AL Date 11/11/21

Personnel receiving samples: MH Second reviewer: MS  
 Personnel labeling samples: MH  
 Project manager notified: MS, MH Date/Time of notification 11/12/2021  
 Name of client notified: \_\_\_\_\_ Date/Time of notification \_\_\_\_\_

## **SAMPLE RESULTS**

## EPA 8015B TPH WATER L-L SGC

AECOM  
1001 Bishop Street, Suite 1600  
Honolulu, HI 96813

APPL Inc.  
908 North Temperance Avenue  
Clovis, CA 93611

Attn: Alethea Ramos

Project: 60571032 CV18F0126 Red Hill Fuel Storage

ARF: 98212

**Sample ID: ERH1907**

**APPL ID: BA46115**

Sample Collection Date: 11/10/21

QCG: #DOC53-211116A1-270744

Method	Analyte	Result	LOQ	LOD	DL	Units	Extraction Date	Analysis Date
EPA 8015B-e	DIESEL (C10-C24)	300.0 U	320	300.0	150.0	ug/L	11/16/21	11/19/21
EPA 8015B-e	OIL (C24-C40)	300.0 U	320	300.0	150.0	ug/L	11/16/21	11/19/21
EPA 8015B-e	SURROGATE: (R) DECANOIC ACID (S)	0.0	0-1			%	11/16/21	11/19/21
EPA 8015B-e	SURROGATE: OCTACOSANE (S)	86.8	60-142			%	11/16/21	11/19/21
EPA 8015B-e	SURROGATE: ORTHO-TERPHENYL (S)	69.2	56-125			%	11/16/21	11/19/21

Quant Method: DEC0911.M
Run #: 1117103
Instrument: Apollo
Sequence: 211117
Dilution Factor: 1
Initials: KAB

Printed: 11/30/2021 9:44:08 AM  
APPL-F1-SC-NoMC-REG MDLs-DOD

## EPA 8015B TPH LIQ-LIQ

AECOM  
1001 Bishop Street, Suite 1600  
Honolulu, HI 96813

Attn: Alethea Ramos

Project: 60571032 CV18F0126 Red Hill Fuel Storage

**Sample ID: ERH1907**

Sample Collection Date: 11/10/21

APPL Inc.  
908 North Temperance Avenue  
Clovis, CA 93611

ARF: 98212

**APPL ID: BA46115**

QCG: #DOC53-211116A-270742

Method	Analyte	Result	LOQ	LOD	DL	Units	Extraction Date	Analysis Date
EPA 8015B-e	DIESEL (C10-C24)	300.0 U	320	300.0	150.0	ug/L	11/16/21	11/19/21
EPA 8015B-e	OIL (C24-C40)	300 B J	320	300.0	150.0	ug/L	11/16/21	11/19/21
EPA 8015B-e	SURROGATE: OCTACOSANE (S)	95.8	60-142			%	11/16/21	11/19/21
EPA 8015B-e	SURROGATE: ORTHO-TERPHENYL (S)	76.7	56-125			%	11/16/21	11/19/21

J = Estimated value.

B = The analyte was found in a method blank, as well as in the sample.

Quant Method: DOC1028.M
Run #: 1117089
Instrument: Apollo
Sequence: 211117
Dilution Factor: 1
Initials: KAB

Printed: 11/30/2021 9:44:08 AM  
APPL-F1-SC-NoMC-REG MDLs-DOD



# EPA 8015B TPH WATER L-L SGC

AECOM  
1001 Bishop Street, Suite 1600  
Honolulu, HI 96813

APPL Inc.  
908 North Temperance Avenue  
Clovis, CA 93611

Attn: Alethea Ramos

Project: 60571032 CV18F0126 Red Hill Fuel Storage

ARF: 98212

**Sample ID: ERH1909**

**APPL ID: BA46116**

Sample Collection Date: 11/10/21

QCG: #DOC53-211116A1-270744

Method	Analyte	Result	LOQ	LOD	DL	Units	Extraction Date	Analysis Date
EPA 8015B-e	DIESEL (C10-C24)	300.0 U	320	300.0	150.0	ug/L	11/16/21	11/19/21
EPA 8015B-e	OIL (C24-C40)	300.0 U	320	300.0	150.0	ug/L	11/16/21	11/19/21
EPA 8015B-e	SURROGATE: (R) DECANOIC ACID (S)	0.0	0-1			%	11/16/21	11/19/21
EPA 8015B-e	SURROGATE: OCTACOSANE (S)	108	60-142			%	11/16/21	11/19/21
EPA 8015B-e	SURROGATE: ORTHO-TERPHENYL (S)	87.4	56-125			%	11/16/21	11/19/21

Quant Method: DEC0911.M
Run #: 1117104
Instrument: Apollo
Sequence: 211117
Dilution Factor: 1
Initials: KAB

Printed: 11/30/2021 9:44:08 AM  
APPL-F1-SC-NoMC-REG MDLs-DOD

## EPA 8015B TPH LIQ-LIQ

AECOM  
1001 Bishop Street, Suite 1600  
Honolulu, HI 96813

Attn: Alethea Ramos

Project: 60571032 CV18F0126 Red Hill Fuel Storage

**Sample ID: ERH1909**

Sample Collection Date: 11/10/21

APPL Inc.  
908 North Temperance Avenue  
Clovis, CA 93611

ARF: 98212

**APPL ID: BA46116**

QCG: #DOC53-211116A-270742

Method	Analyte	Result	LOQ	LOD	DL	Units	Extraction Date	Analysis Date
EPA 8015B-e	DIESEL (C10-C24)	300.0 U	320	300.0	150.0	ug/L	11/16/21	11/19/21
EPA 8015B-e	OIL (C24-C40)	270 B J	320	300.0	150.0	ug/L	11/16/21	11/19/21
EPA 8015B-e	SURROGATE: OCTACOSANE (S)	94.7	60-142			%	11/16/21	11/19/21
EPA 8015B-e	SURROGATE: ORTHO-TERPHENYL (S)	75.7	56-125			%	11/16/21	11/19/21

J = Estimated value.

B = The analyte was found in a method blank, as well as in the sample.

Quant Method: DOC1028.M
Run #: 1117090
Instrument: Apollo
Sequence: 211117
Dilution Factor: 1
Initials: KAB

Printed: 11/30/2021 9:44:08 AM  
APPL-F1-SC-NoMC-REG MDLs-DOD

# EPA 8015B TPH LIQ-LIQ

AECOM  
1001 Bishop Street, Suite 1600  
Honolulu, HI 96813

Attn: Alethea Ramos

Project: 60571032 CV18F0126 Red Hill Fuel Storage

**Sample ID: ERH1907 BLANK**

Sample Collection Date: 11/10/21

APPL Inc.  
908 North Temperance Avenue  
Clovis, CA 93611

ARF: 98212

**APPL ID: BA46118**

QCG: #RHBLK-211115A-270717

Method	Analyte	Result	LOQ	LOD	DL	Units	Extraction Date	Analysis Date
EPA 8015B-e	DIESEL (C10-C24)	300.0 U	320	300.0	150.0	ug/L	11/15/21	11/18/21
EPA 8015B-e	OIL (C24-C40)	300.0 U	320	300.0	150.0	ug/L	11/15/21	11/18/21
EPA 8015B-e	SURROGATE: OCTACOSANE (S)	62.5	60-142			%	11/15/21	11/18/21
EPA 8015B-e	SURROGATE: ORTHO-TERPHENYL (S)	50.6 #	56-125			%	11/15/21	11/18/21

# = Recovery (or RPD) is outside QC limits.

Quant Method: DOC1028.M  
Run #: 1117037  
Instrument: Apollo  
Sequence: 211117  
Dilution Factor: 1  
Initials: KAB

Printed: 11/30/2021 9:44:08 AM  
APPL-F1-SC-NoMC-REG MDLs-DOD

# EPA 8015B TPH LIQ-LIQ

AECOM  
1001 Bishop Street, Suite 1600  
Honolulu, HI 96813

Attn: Alethea Ramos

Project: 60571032 CV18F0126 Red Hill Fuel Storage

**Sample ID: ERH1909 BLANK**

Sample Collection Date: 11/10/21

APPL Inc.  
908 North Temperance Avenue  
Clovis, CA 93611

ARF: 98212

**APPL ID: BA46119**

QCG: #RHBLK-211115A-270717

Method	Analyte	Result	LOQ	LOD	DL	Units	Extraction Date	Analysis Date
EPA 8015B-e	DIESEL (C10-C24)	300.0 U	320	300.0	150.0	ug/L	11/15/21	11/18/21
EPA 8015B-e	OIL (C24-C40)	300.0 U	320	300.0	150.0	ug/L	11/15/21	11/18/21
EPA 8015B-e	SURROGATE: OCTACOSANE (S)	88.4	60-142			%	11/15/21	11/18/21
EPA 8015B-e	SURROGATE: ORTHO-TERPHENYL (S)	70.8	56-125			%	11/15/21	11/18/21

Quant Method: DOC1028.M  
Run #: 1117038  
Instrument: Apollo  
Sequence: 211117  
Dilution Factor: 1  
Initials: KAB

Printed: 11/30/2021 9:44:08 AM  
APPL-F1-SC-NoMC-REG MDLs-DOD

# EPA 8270D SIM LIQ-LIQ

AECOM  
1001 Bishop Street, Suite 1600  
Honolulu, HI 96813

APPL Inc.  
908 North Temperance Avenue  
Clovis, CA 93611

Attn: Alethea Ramos

Project: 60571032 CV18F0126 Red Hill Fuel Storage

ARF: 98212

**Sample ID: ERH1907**

**APPL ID: BA46115**

Sample Collection Date: 11/10/21

QCG: #SIM53-211115AK-271047

Method	Analyte	Result	LOQ	LOD	DL	Units	Extraction Date	Analysis Date
8270D-SIM	1-METHYLNAPHTHALENE	0.10 U	0.2	0.10	0.04	ug/L	11/15/21	11/18/21
8270D-SIM	2-METHYLNAPHTHALENE	0.10 U	0.2	0.10	0.04	ug/L	11/15/21	11/18/21
8270D-SIM	NAPHTHALENE	0.10 U	0.2	0.10	0.04	ug/L	11/15/21	11/18/21
8270D-SIM	SURROGATE: 2-METHYLNAPHTHALEN	85.3	39-114			%	11/15/21	11/18/21
8270D-SIM	SURROGATE: FLUORANTHENE-D10 (S	98.4	58-120			%	11/15/21	11/18/21

Quant Method: K1019.M
Run #: 1019K448
Instrument: KYLO
Sequence: 211019
Dilution Factor: 1
Initials: LSI

Printed: 11/30/2021 1:06:42 PM  
APPL-F1-SC-NoMC-REG MDLs-DOD

# EPA 8270D SIM LIQ-LIQ

AECOM  
1001 Bishop Street, Suite 1600  
Honolulu, HI 96813

APPL Inc.  
908 North Temperance Avenue  
Clovis, CA 93611

Attn: Alethea Ramos  
Project: 60571032 CV18F0126 Red Hill Fuel Storage

ARF: 98212  
**APPL ID: BA46116**  
QCG: #SIM53-211115AK-271047

**Sample ID: ERH1909**

Sample Collection Date: 11/10/21

Method	Analyte	Result	LOQ	LOD	DL	Units	Extraction Date	Analysis Date
8270D-SIM	1-METHYLNAPHTHALENE	0.10 U	0.2	0.10	0.04	ug/L	11/15/21	11/18/21
8270D-SIM	2-METHYLNAPHTHALENE	0.10 U	0.2	0.10	0.04	ug/L	11/15/21	11/18/21
8270D-SIM	NAPHTHALENE	0.10 U	0.2	0.10	0.04	ug/L	11/15/21	11/18/21
8270D-SIM	SURROGATE: 2-METHYLNAPHTHALEN	94.0	39-114			%	11/15/21	11/18/21
8270D-SIM	SURROGATE: FLUORANTHENE-D10 (S	100	58-120			%	11/15/21	11/18/21

Quant Method: K1019.M
Run #: 1019K449
Instrument: KYLO
Sequence: 211019
Dilution Factor: 1
Initials: LSI

Printed: 11/30/2021 1:06:42 PM  
APPL-F1-SC-NoMC-REG MDLs-DOD

## EPA 8260B BTEX WATER

AECOM  
1001 Bishop Street, Suite 1600  
Honolulu, HI 96813

Attn: Alethea Ramos  
Project: 60571032 CV18F0126 Red Hill Fuel Storage

**Sample ID: ERH1906**

Sample Collection Date: 11/10/21

APPL Inc.  
908 North Temperance Avenue  
Clovis, CA 93611

ARF: 98212

**APPL ID: BA46114**

QCG: #86BTO-AM211115-270528

Method	Analyte	Result	LOQ	LOD	DL	Units	Extraction Date	Analysis Date
EPA 8260B	BENZENE	0.30 U	1.0	0.30	0.15	ug/L	11/15/21	11/15/21
EPA 8260B	ETHYLBENZENE	0.50 U	1.0	0.50	0.23	ug/L	11/15/21	11/15/21
EPA 8260B	TOLUENE	0.30 U	1.0	0.30	0.15	ug/L	11/15/21	11/15/21
EPA 8260B	XYLENES (TOTAL)	0.30 U	2.0	0.30	0.15	ug/L	11/15/21	11/15/21
EPA 8260B	SURROGATE: 1,2-DICHLOROETHANE-	104	81-118			%	11/15/21	11/15/21
EPA 8260B	SURROGATE: 4-BROMOFLUOROBENZ	101	85-114			%	11/15/21	11/15/21
EPA 8260B	SURROGATE: DIBROMOFLUOROMETH	106	80-119			%	11/15/21	11/15/21
EPA 8260B	SURROGATE: TOLUENE-D8 (S)	98.1	89-112			%	11/15/21	11/15/21

Quant Method: M1111W.M  
Run #: 1115M12  
Instrument: Max  
Sequence: 211111  
Dilution Factor: 1  
Initials: PAN

Printed: 11/22/2021 1:08:31 PM  
APPL-F1-SC-NoMC-REG MDLs-DOD

## EPA 8260B BTEX WATER

AECOM  
1001 Bishop Street, Suite 1600  
Honolulu, HI 96813

Attn: Alethea Ramos

Project: 60571032 CV18F0126 Red Hill Fuel Storage

**Sample ID: ERH1907**

Sample Collection Date: 11/10/21

APPL Inc.  
908 North Temperance Avenue  
Clovis, CA 93611

ARF: 98212

**APPL ID: BA46115**

QCG: #86BTO-AM211115-270528

Method	Analyte	Result	LOQ	LOD	DL	Units	Extraction Date	Analysis Date
EPA 8260B	BENZENE	0.30 U	1.0	0.30	0.15	ug/L	11/15/21	11/15/21
EPA 8260B	ETHYLBENZENE	0.50 U	1.0	0.50	0.23	ug/L	11/15/21	11/15/21
EPA 8260B	TOLUENE	0.30 U	1.0	0.30	0.15	ug/L	11/15/21	11/15/21
EPA 8260B	XYLENES (TOTAL)	0.30 U	2.0	0.30	0.15	ug/L	11/15/21	11/15/21
EPA 8260B	SURROGATE: 1,2-DICHLOROETHANE-	104	81-118			%	11/15/21	11/15/21
EPA 8260B	SURROGATE: 4-BROMOFLUOROBENZ	98.8	85-114			%	11/15/21	11/15/21
EPA 8260B	SURROGATE: DIBROMOFLUOROMETH	107	80-119			%	11/15/21	11/15/21
EPA 8260B	SURROGATE: TOLUENE-D8 (S)	99.5	89-112			%	11/15/21	11/15/21

Quant Method: M1111W.M  
Run #: 1115M13  
Instrument: Max  
Sequence: 211111  
Dilution Factor: 1  
Initials: PAN

Printed: 11/22/2021 1:08:31 PM  
APPL-F1-SC-NoMC-REG MDLs-DOD



# EPA 8260B BTEX WATER

AECOM  
1001 Bishop Street, Suite 1600  
Honolulu, HI 96813

Attn: Alethea Ramos

Project: 60571032 CV18F0126 Red Hill Fuel Storage

**Sample ID: ERH1909**

Sample Collection Date: 11/10/21

APPL Inc.  
908 North Temperance Avenue  
Clovis, CA 93611

ARF: 98212

**APPL ID: BA46116**

QCG: #86BTO-AM211115-270528

Method	Analyte	Result	LOQ	LOD	DL	Units	Extraction Date	Analysis Date
EPA 8260B	BENZENE	0.30 U	1.0	0.30	0.15	ug/L	11/15/21	11/15/21
EPA 8260B	ETHYLBENZENE	0.50 U	1.0	0.50	0.23	ug/L	11/15/21	11/15/21
EPA 8260B	TOLUENE	0.30 U	1.0	0.30	0.15	ug/L	11/15/21	11/15/21
EPA 8260B	XYLENES (TOTAL)	0.30 U	2.0	0.30	0.15	ug/L	11/15/21	11/15/21
EPA 8260B	SURROGATE: 1,2-DICHLOROETHANE-	104	81-118			%	11/15/21	11/15/21
EPA 8260B	SURROGATE: 4-BROMOFLUOROBENZ	95.3	85-114			%	11/15/21	11/15/21
EPA 8260B	SURROGATE: DIBROMOFLUOROMETH	107	80-119			%	11/15/21	11/15/21
EPA 8260B	SURROGATE: TOLUENE-D8 (S)	94.4	89-112			%	11/15/21	11/15/21

Quant Method: M1111W.M  
Run #: 1115M14  
Instrument: Max  
Sequence: 211111  
Dilution Factor: 1  
Initials: PAN

Printed: 11/22/2021 1:08:31 PM  
APPL-F1-SC-NoMC-REG MDLs-DOD

# EPA 8260B GRO WATER

AECOM  
1001 Bishop Street, Suite 1600  
Honolulu, HI 96813

Attn: Alethea Ramos  
Project: 60571032 CV18F0126 Red Hill Fuel Storage

**Sample ID: ERH1906**

Sample Collection Date: 11/10/21

APPL Inc.  
908 North Temperance Avenue  
Clovis, CA 93611

ARF: 98212

**APPL ID: BA46114**

QCG: #GRO86-211115AM-270843

Method	Analyte	Result	LOQ	LOD	DL	Units	Extraction Date	Analysis Date
EPA 8260B	GASOLINE RANGE ORGANICS	18.0 U	20	18.0	8.6	ug/L	11/15/21	11/15/21
EPA 8260B	SURROGATE: 4-BROMOFLUOROBENZ	100.0	85-114			%	11/15/21	11/15/21

Quant Method: MGAS0825.M  
Run #: 1115M12  
Instrument: Max  
Sequence: 211111  
Dilution Factor: 1  
Initials: PAN

Printed: 11/23/2021 9:05:41 AM  
APPL-F1-SC-NoMC-REG MDLs-DOD

# EPA 8260B GRO WATER

AECOM  
1001 Bishop Street, Suite 1600  
Honolulu, HI 96813

Attn: Alethea Ramos  
Project: 60571032 CV18F0126 Red Hill Fuel Storage

**Sample ID: ERH1907**

Sample Collection Date: 11/10/21

APPL Inc.  
908 North Temperance Avenue  
Clovis, CA 93611

ARF: 98212

**APPL ID: BA46115**

QCG: #GRO86-211115AM-270843

Method	Analyte	Result	LOQ	LOD	DL	Units	Extraction Date	Analysis Date
EPA 8260B	GASOLINE RANGE ORGANICS	18.0 U	20	18.0	8.6	ug/L	11/15/21	11/15/21
EPA 8260B	SURROGATE: 4-BROMOFLUOROBENZ	97.8	85-114			%	11/15/21	11/15/21

Quant Method: MGAS0825.M  
Run #: 1115M13  
Instrument: Max  
Sequence: 211111  
Dilution Factor: 1  
Initials: PAN

Printed: 11/23/2021 9:05:41 AM  
APPL-F1-SC-NoMC-REG MDLs-DOD

# EPA 8260B GRO WATER

AECOM  
1001 Bishop Street, Suite 1600  
Honolulu, HI 96813

Attn: Alethea Ramos  
Project: 60571032 CV18F0126 Red Hill Fuel Storage

**Sample ID: ERH1909**

Sample Collection Date: 11/10/21

APPL Inc.  
908 North Temperance Avenue  
Clovis, CA 93611

ARF: 98212

**APPL ID: BA46116**

QCG: #GRO86-211115AM-270843

Method	Analyte	Result	LOQ	LOD	DL	Units	Extraction Date	Analysis Date
EPA 8260B	GASOLINE RANGE ORGANICS	18.0 U	20	18.0	8.6	ug/L	11/15/21	11/15/21
EPA 8260B	SURROGATE: 4-BROMOFLUOROBENZ	94.4	85-114			%	11/15/21	11/15/21

Quant Method: MGAS0825.M  
Run #: 1115M14  
Instrument: Max  
Sequence: 211111  
Dilution Factor: 1  
Initials: PAN

Printed: 11/23/2021 9:05:41 AM  
APPL-F1-SC-NoMC-REG MDLs-DOD

## Wet Lab Analysis

AECOM  
1001 Bishop Street, Suite 1600  
Honolulu, HI 96813

APPL Inc.  
908 North Temperance Avenue  
Clovis, CA 93611

Attn: Alethea Ramos  
Project: 60571032 CV18F0126 Red Hill Fuel Storage

**Sample ID: ERH1907**  
Sample Collection Date: 11/10/2021

**APPL ID: BA46115**  
ARF: 98212

Method	Analyte	Result	LOQ	LOD	DL	Units	DF	Prep Date	Analysis Date
SW846 9060A	TOTAL ORGANIC CARBON	0.19 J	0.93	0.350	0.130	mg/L	1	11/20/21	11/20/21

J = Estimated value.

Printed: 11/24/2021 10:21:24 AM

APPL-F1-SC-NoMC-REG MDLs

# QC FORMS

# EPA 8015B-eHL

Form 2 & 8

## Surrogate Recovery

Lab Name: APPL, Inc.  
Case No: 98212  
Matrix: WATER

SDG No: 98212  
Date Analyzed: 11/18/2021  
Instrument: Apollo

APPL ID.	Client Sample No.	SURROGATE: OCTACOSANE (S)			SURROGATE: ORTHO-TERPHENYL (S)		
		Limits	Result	Qualifier	Limits	Result	Qualifier
211116A-BLK	Blank	60-142	90.8		56-125	73.1	
211116A-LCS	Lab Control Spike	60-142	94.7		56-125	86.0	
211116A-LCSD	Lab Control SpikeD	60-142	94.7		56-125	85.3	
BA46115	ERH1907	60-142	95.8		56-125	76.7	
BA46116	ERH1909	60-142	94.7		56-125	75.7	
BA46117	ERH1915	60-142	99.3		56-125	79.5	

Comments: Batch: #DOC53-211116A

Printed: 11/19/2021 7:38:54 PM  
Form 2 & 8, Surrogate Recovery Summary

# EPA 8015B-eHL

Form 2 & 8

## Surrogate Recovery

Lab Name: APPL, Inc.  
Case No: 98212  
Matrix: WATER

SDG No: 98212  
Date Analyzed: 11/19/2021  
Instrument: Apollo

APPL ID.	Client Sample No.	SURROGATE: (R) DECANOIC ACID (S)			SURROGATE: OCTACOSANE (S)		
		Limits	Result	Qualifier	Limits	Result	Qualifier
211116A1-BLK	Blank	0-1	0.0		60-142	117	
211116A1-LCS	Lab Control Spike	0-1	0.0		60-142	124	
211116A1-LCSD	Lab Control SpikeD	0-1	0.0		60-142	111	
BA46115	ERH1907	0-1	0.0		60-142	86.8	
BA46116	ERH1909	0-1	0.0		60-142	108	
BA46117	ERH1915	0-1	0.0		60-142	94.1	

Comments: Batch: #DOC53-211116A1

Printed: 11/19/2021 7:38:54 PM  
Form 2 & 8, Surrogate Recovery Summary



# EPA 8015B-eHL

Form 2 & 8

## Surrogate Recovery

Lab Name: APPL, Inc.

SDG No: 98212

Case No: 98212

Date Analyzed: 11/19/2021

Matrix: WATER

Instrument: Apollo

APPL ID.	Client Sample No.	SURROGATE: ORTHO-TERPHENYL					
		(S)					
		Limits	Result	Qualifier	Limits	Result	Qualifier
211116A1-BLK	Blank	56-125	92.8				
211116A1-LCS	Lab Control Spike	56-125	112				
211116A1-LCSD	Lab Control SpikeD	56-125	95.3				
BA46115	ERH1907	56-125	69.2				
BA46116	ERH1909	56-125	87.4				
BA46117	ERH1915	56-125	75.6				

Comments: Batch: #DOC53-211116A1

Printed: 11/19/2021 7:38:54 PM  
Form 2 & 8, Surrogate Recovery Summary

# EPA 8015B-eHL

Form 2 & 8

## Surrogate Recovery

Lab Name: APPL, Inc.  
Case No: 98212  
Matrix: WATER

SDG No: 98212  
Date Analyzed: 11/17/2021  
Instrument: Apollo

APPL ID.	Client Sample No.	SURROGATE: OCTACOSANE (S)			SURROGATE: ORTHO-TERPHENYL (S)		
		Limits	Result	Qualifier	Limits	Result	Qualifier
211115A-BLK	Blank	60-142	87.1		56-125	69.2	
211115A-LCS	Lab Control Spike	60-142	88.0		56-125	70.7	
211115A-LCSD	Lab Control SpikeD	60-142	84.0		56-125	67.3	
BA46118	ERH1907 BLANK	60-142	62.5		56-125	50.6	#
BA46119	ERH1909 BLANK	60-142	88.4		56-125	70.8	
BA46120	ERH1915 BLANK	60-142	79.6		56-125	64.3	

Comments: Batch: #RHBLK-211115A  
# = Recovery outside of Control Limits on Sample.

Printed: 11/19/2021 7:38:54 PM  
Form 2 & 8, Surrogate Recovery Summary

# EPA 8015B-eH

Form 4

## Blank Summary

Lab Name: APPL, Inc.

SDG No: 98212

Case No: 98212

Date Analyzed: 11/18/2021

Matrix: WATER

Instrument: Apollo

Blank ID: 211116A-BLK

Time Analyzed: 2317

<b>APPL ID.</b>	<b>Client Sample No.</b>	<b>File ID.</b>	<b>Date Analyzed</b>
211116A-BLK	Blank	1117081	11/18/2021 2317
211116A-LCS	Lab Control Spike	1117082	11/18/2021 2345
211116A-LCSD	Lab Control Spiked	1117083	11/19/2021 0013
BA46115	ERH1907	1117089	11/19/2021 0301
BA46116	ERH1909	1117090	11/19/2021 0330
BA46117	ERH1915	1117091	11/19/2021 0358

Comments: Batch: #DOC53-211116A

Printed: 11/19/2021 7:38:46 PM  
Form 4, Blank Summary

# EPA 8015B-eH

Form 4

## Blank Summary

Lab Name: APPL, Inc.

SDG No: 98212

Case No: 98212

Date Analyzed: 11/19/2021

Matrix: WATER

Instrument: Apollo

Blank ID: 211116A1-BLK

Time Analyzed: 0550

<b>APPL ID.</b>	<b>Client Sample No.</b>	<b>File ID.</b>	<b>Date Analyzed</b>
211116A1-BLK	Blank	1117095	11/19/2021 0550
211116A1-LCS	Lab Control Spike	1117096	11/19/2021 0618
211116A1-LCSD	Lab Control Spiked	1117097	11/19/2021 0646
BA46115	ERH1907	1117103	11/19/2021 0934
BA46116	ERH1909	1117104	11/19/2021 1002
BA46117	ERH1915	1117105	11/19/2021 1030

Comments: Batch: #DOC53-211116A1

Printed: 11/19/2021 7:38:46 PM  
Form 4, Blank Summary

# EPA 8015B-eH

Form 4

## Blank Summary

Lab Name: APPL, Inc.

SDG No: 98212

Case No: 98212

Date Analyzed: 11/17/2021

Matrix: WATER

Instrument: Apollo

Blank ID: 211115A-BLK

Time Analyzed: 2255

<b>APPL ID.</b>	<b>Client Sample No.</b>	<b>File ID.</b>	<b>Date Analyzed</b>
211115A-BLK	Blank	1117029	11/17/2021 2255
211115A-LCS	Lab Control Spike	1117030	11/17/2021 2323
211115A-LCSD	Lab Control Spiked	1117031	11/17/2021 2351
BA46118	ERH1907 BLANK	1117037	11/18/2021 0239
BA46119	ERH1909 BLANK	1117038	11/18/2021 0308
BA46120	ERH1915 BLANK	1117040	11/18/2021 0404

Comments: Batch: #RHBLK-211115A

Printed: 11/19/2021 7:38:46 PM  
Form 4, Blank Summary

**Method Blank**  
**EPA 8015B TPH LIQ-LIQ**

Blank Name/QCG: **211115W-46002 - 270717**  
Batch ID: #RHBLK-211115A

APPL Inc.  
908 North Temperance Avenue  
Clovis, CA 93611

Sample Type	Analyte	Result	LOQ	LOD	DL	Units	Extraction Date	Analysis Date
BLANK	DIESEL (C10-C24)	300.0 U	320	300.0	150.0	ug/L	11/15/2021	11/17/2021
BLANK	OIL (C24-C40)	300.0 U	320	300.0	150.0	ug/L	11/15/2021	11/17/2021
BLANK	SURROGATE: OCTACOSANE (S)	87.1	60-142			%	11/15/2021	11/17/2021
BLANK	SURROGATE: ORTHO-TERPHEN	69.2	56-125			%	11/15/2021	11/17/2021

Quant Method:DOC1028.M  
Run #:1117029  
Instrument:Apollo  
Sequence:211117  
Initials:KAB

GC SC-Blank-REG MDLs-DOD  
Printed: 11/19/2021 7:39:05 PM

**Method Blank**  
**EPA 8015B TPH LIQ-LIQ**

Blank Name/QCG: **211116W-46001 - 270742**  
Batch ID: #DOC53-211116A

APPL Inc.  
908 North Temperance Avenue  
Clovis, CA 93611

Sample Type	Analyte	Result	LOQ	LOD	DL	Units	Extraction Date	Analysis Date
BLANK	DIESEL (C10-C24)	300.0 U	320	300.0	150.0	ug/L	11/16/2021	11/18/2021
BLANK	OIL (C24-C40)	340	320	300.0	150.0	ug/L	11/16/2021	11/18/2021
BLANK	SURROGATE: OCTACOSANE (S)	90.8	60-142			%	11/16/2021	11/18/2021
BLANK	SURROGATE: ORTHO-TERPHEN	73.1	56-125			%	11/16/2021	11/18/2021

Quant Method:DOC1028.M  
Run #:1117081  
Instrument:Apollo  
Sequence:211117  
Initials:KAB

GC SC-Blank-REG MDLs-DOD  
Printed: 11/19/2021 7:39:05 PM

**Method Blank**  
**EPA 8015B TPH WATER L-L SGC**

Blank Name/QCG: **211116W-46001 - 270744**  
Batch ID: #DOC53-211116A1

APPL Inc.  
908 North Temperance Avenue  
Clovis, CA 93611

Sample Type	Analyte	Result	LOQ	LOD	DL	Units	Extraction Date	Analysis Date
BLANK	DIESEL (C10-C24)	300.0 U	320	300.0	150.0	ug/L	11/16/2021	11/19/2021
BLANK	OIL (C24-C40)	260 J	320	300.0	150.0	ug/L	11/16/2021	11/19/2021
BLANK	SURROGATE: (R) DECANOIC AC	0.0	0-1			%	11/16/2021	11/19/2021
BLANK	SURROGATE: OCTACOSANE (S)	117	60-142			%	11/16/2021	11/19/2021
BLANK	SURROGATE: ORTHO-TERPHEN	92.8	56-125			%	11/16/2021	11/19/2021

J = Estimated value.

Quant Method: DEC0911.M  
Run #: 1117095  
Instrument: Apollo  
Sequence: 211117  
Initials: KAB

GC SC-Blank-REG MDLs-DOD  
Printed: 11/30/2021 9:44:30 AM



# EPA 8015B-eH

Form 4

## LCS Summary

Lab Name: APPL, Inc.

SDG No: 98212

Case No: 98212

Date Analyzed: 11/18/2021

Matrix: WATER

Instrument: Apollo

LCS ID: 211116A-LCS

Time Analyzed: 2345

<b>APPL ID.</b>	<b>Client Sample No.</b>	<b>File ID.</b>	<b>Date Analyzed</b>
211116A-BLK	Blank	1117081	11/18/2021 2317
211116A-LCS	Lab Control Spike	1117082	11/18/2021 2345
211116A-LCSD	Lab Control Spiked	1117083	11/19/2021 0013
BA46115	ERH1907	1117089	11/19/2021 0301
BA46116	ERH1909	1117090	11/19/2021 0330
BA46117	ERH1915	1117091	11/19/2021 0358

Comments: Batch: #DOC53-211116A

Printed: 11/19/2021 7:38:44 PM  
Form 4, LCS Summary

# EPA 8015B-eH

Form 4

## LCS Summary

Lab Name: APPL, Inc.

SDG No: 98212

Case No: 98212

Date Analyzed: 11/19/2021

Matrix: WATER

Instrument: Apollo

LCS ID: 211116A1-LCS

Time Analyzed: 0618

<b>APPL ID.</b>	<b>Client Sample No.</b>	<b>File ID.</b>	<b>Date Analyzed</b>
211116A1-BLK	Blank	1117095	11/19/2021 0550
211116A1-LCS	Lab Control Spike	1117096	11/19/2021 0618
211116A1-LCSD	Lab Control Spiked	1117097	11/19/2021 0646
BA46115	ERH1907	1117103	11/19/2021 0934
BA46116	ERH1909	1117104	11/19/2021 1002
BA46117	ERH1915	1117105	11/19/2021 1030

Comments: Batch: #DOC53-211116A1

Printed: 11/19/2021 7:38:44 PM  
Form 4, LCS Summary

# EPA 8015B-eH

Form 4

## LCS Summary

Lab Name: APPL, Inc.

SDG No: 98212

Case No: 98212

Date Analyzed: 11/17/2021

Matrix: WATER

Instrument: Apollo

LCS ID: 211115A-LCS

Time Analyzed: 2323

<b>APPL ID.</b>	<b>Client Sample No.</b>	<b>File ID.</b>	<b>Date Analyzed</b>	
211115A-BLK	Blank	1117029	11/17/2021	2255
211115A-LCS	Lab Control Spike	1117030	11/17/2021	2323
211115A-LCSD	Lab Control Spiked	1117031	11/17/2021	2351
BA46118	ERH1907 BLANK	1117037	11/18/2021	0239
BA46119	ERH1909 BLANK	1117038	11/18/2021	0308
BA46120	ERH1915 BLANK	1117040	11/18/2021	0404

Comments: Batch: #RHBLK-211115A

Printed: 11/19/2021 7:38:44 PM  
Form 4, LCS Summary

## Laboratory Control Spike Recoveries

### EPA 8015B TPH LIQ-LIQ

APPL ID: 211116W-46001 LCS - 270742

Batch ID: #DOC53-211116A

APPL Inc.

908 North Temperance Avenue

Clovis, CA 93611

Compound Name	Spike Lvl ug/L	SPK Result ug/L	DUP Result ug/L	SPK % Recovery	DUP % Recovery	Recovery Limits	RPD %	RPD Limits
DIESEL (C10-C24)	2000	1840	1770	92.0	88.5	36-132	3.9	30
OIL (C24-C40)	2000	1890	1900	94.5	95.0	41-113	0.53	30
-----								
SURROGATE: OCTACOSANE (S)	150	142	142	94.7	94.7	60-142		
SURROGATE: ORTHO-TERPHENYL (S)	150	129	128	86.0	85.3	56-125		
-----								

Comments: \_\_\_\_\_

<u>Primary</u>	<u>SPK</u>	<u>DUP</u>
Quant Method :	DOC1028.M	DOC1028.M
Extraction Date :	11/16/2021	11/16/2021
Analysis Date :	11/18/2021	11/19/2021
Instrument :	Apollo	Apollo
Run :	1117082	1117083
Initials :	KAB	

## Laboratory Control Spike Recoveries

### EPA 8015B TPH WATER L-L SGC

APPL ID: 211116W-46001 LCS - 270744

Batch ID: #DOC53-211116A1

APPL Inc.

908 North Temperance Avenue

Clovis, CA 93611

Compound Name	Spike Lvl ug/L	SPK Result ug/L	DUP Result ug/L	SPK % Recovery	DUP % Recovery	Recovery Limits	RPD %	RPD Limits
DIESEL (C10-C24)	2000	2300	1940	115	97.0	36-132	17.0	30
OIL (C24-C40)	2000	2460	2220	123 #	111	41-113	10.3	30
SURROGATE: (R) DECANOIC ACID (S)	10.00	0	0	0.0	0.0	0-1		
SURROGATE: OCTACOSANE (S)	150	186	167	124	111	60-142		
SURROGATE: ORTHO-TERPHENYL (S)	150	168	143	112	95.3	56-125		

# = Recovery is outside QC limits.

Comments:

<u>Primary</u>	<u>SPK</u>	<u>DUP</u>
Quant Method :	DEC0911.M	DEC0911.M
Extraction Date :	11/16/2021	11/16/2021
Analysis Date :	11/19/2021	11/19/2021
Instrument :	Apollo	Apollo
Run :	1117096	1117097
Initials :	KAB	

# Laboratory Control Spike Recoveries

## EPA 8015B TPH LIQ-LIQ

APPL ID: 211115W-46002 LCS - 270717  
 Batch ID: #RHBLK-211115A

APPL Inc.  
 908 North Temperance Avenue  
 Clovis, CA 93611

Compound Name	Spike Lvl ug/L	SPK Result ug/L	DUP Result ug/L	SPK % Recovery	DUP % Recovery	Recovery Limits	RPD %	RPD Limits
DIESEL (C10-C24)	0	45.8	46.1	NA	NA	36-132		30
OIL (C24-C40)	0	45.8	49.5	NA	NA	41-113		30
-----								
SURROGATE: OCTACOSANE (S)	150	132	126	88.0	84.0	60-142		
SURROGATE: ORTHO-TERPHENYL (S)	150	106	101	70.7	67.3	56-125		
-----								

Comments: \_\_\_\_\_

<u>Primary</u>	<u>SPK</u>	<u>DUP</u>
Quant Method :	DOC1028.M	DOC1028.M
Extraction Date :	11/15/2021	11/15/2021
Analysis Date :	11/17/2021	11/17/2021
Instrument :	Apollo	Apollo
Run :	1117030	1117031
Initials :	KAB	

# 8270D-SIM

Form 2 & 8

## Surrogate Recovery

Lab Name: APPL, Inc.

SDG No: 98212

Case No: 98212

Date Analyzed: 11/18/2021

Matrix: WATER

Instrument: KYLO

APPL ID.	Client Sample No.	SURROGATE: 2-METHYLNAPHTHALENE-D10 (S)			SURROGATE: FLUORANTHENE-D10 (S)		
		Limits	Result	Qualifier	Limits	Result	Qualifier
211115AK-BLK	Blank	39-114	85.7		58-120	101	
211115AK-LCS	Lab Control Spike	39-114	90.2		58-120	101	
211115AK-LCSD	Lab Control SpikeD	39-114	88.4		58-120	96.6	
BA46115	ERH1907	39-114	85.3		58-120	98.4	
BA46116	ERH1909	39-114	94.0		58-120	100	
BA46117	ERH1915	39-114	89.7		58-120	96.8	

Comments: Batch: #SIM53-211115AK

Printed: 11/30/2021 1:06:38 PM  
Form 2 & 8, Surrogate Recovery Summary

# 8270D-SIM

Form 4

## Blank Summary

Lab Name: APPL, Inc.

SDG No: 98212

Case No: 98212

Date Analyzed: 11/18/2021

Matrix: WATER

Instrument: KYLO

Blank ID: 211115AK-BLK

Time Analyzed: 0921

APPL ID.	Client Sample No.	File ID.	Date Analyzed
211115AK-BLK	Blank	1019K438	11/18/2021 0921
211115AK-LCS	Lab Control Spike	1019K439	11/18/2021 0940
211115AK-LCSD	Lab Control Spiked	1019K440	11/18/2021 1000
BA46115	ERH1907	1019K448	11/18/2021 1240
BA46116	ERH1909	1019K449	11/18/2021 1300
BA46117	ERH1915	1019K450	11/18/2021 1320

Comments: Batch: #SIM53-211115AK

Printed: 11/30/2021 1:06:36 PM  
Form 4, Blank Summary



**Method Blank**  
**EPA 8270D SIM LIQ-LIQ**

Blank Name/QCG: **211115W-45998 - 271047**  
Batch ID: #SIM53-211115AK

APPL Inc.  
908 North Temperance Avenue  
Clovis, CA 93611

Sample Type	Analyte	Result	LOQ	LOD	DL	Units	Extraction Date	Analysis Date
BLANK	1-METHYLNAPHTHALENE	0.10 U	0.2	0.10	0.04	ug/L	11/15/2021	11/18/2021
BLANK	2-METHYLNAPHTHALENE	0.10 U	0.2	0.10	0.04	ug/L	11/15/2021	11/18/2021
BLANK	NAPHTHALENE	0.10 U	0.2	0.10	0.04	ug/L	11/15/2021	11/18/2021
BLANK	SURROGATE: 2-METHYLNAPHT	85.7	39-114			%	11/15/2021	11/18/2021
BLANK	SURROGATE: FLUORANTHENE-	101	58-120			%	11/15/2021	11/18/2021

Quant Method:K1019.M  
Run #: 1019K438  
Instrument:KYLO  
Sequence:211019  
Initials:LSI

GC SC-Blank-REG MDLs-DOD  
Printed: 11/30/2021 1:06:45 PM

# **8270D-SIM**

Form 4

## **LCS Summary**

Lab Name: APPL, Inc.

SDG No: 98212

Case No: 98212

Date Analyzed: 11/18/2021

Matrix: WATER

Instrument: KYLO

LCS ID: 211115AK-LCS

Time Analyzed: 0940

<b>APPL ID.</b>	<b>Client Sample No.</b>	<b>File ID.</b>	<b>Date Analyzed</b>
211115AK-BLK	Blank	1019K438	11/18/2021 0921
211115AK-LCS	Lab Control Spike	1019K439	11/18/2021 0940
211115AK-LCSD	Lab Control Spiked	1019K440	11/18/2021 1000
BA46115	ERH1907	1019K448	11/18/2021 1240
BA46116	ERH1909	1019K449	11/18/2021 1300
BA46117	ERH1915	1019K450	11/18/2021 1320

Comments: Batch: #SIM53-211115AK

Printed: 11/30/2021 1:06:34 PM  
Form 4, LCS Summary

**Laboratory Control Spike Recoveries**  
**EPA 8270D SIM LIQ-LIQ**

APPL ID: 211115W-45998 LCS - 271047

Batch ID: #SIM53-211115AK

APPL Inc.

908 North Temperance Avenue

Clovis, CA 93611

Compound Name	Spike Lvl ug/L	SPK Result ug/L	DUP Result ug/L	SPK % Recovery	DUP % Recovery	Recovery Limits	RPD %	RPD Limits
1-METHYLNAPHTHALENE	5.00	4.04	3.65	80.8	73.0	41-115	10.1	20
2-METHYLNAPHTHALENE	5.00	4.07	3.71	81.4	74.2	39-114	9.3	20
NAPHTHALENE	5.00	3.98	3.63	79.6	72.6	43-114	9.2	20
-----								
SURROGATE: 2-METHYLNAPHTHALEN	5.00	4.51	4.42	90.2	88.4	39-114		
SURROGATE: FLUORANTHENE-D10 (S)	5.00	5.05	4.83	101	96.6	58-120		
-----								

Comments: \_\_\_\_\_

<u>Primary</u>	<u>SPK</u>	<u>DUP</u>
Quant Method :	K1019.M	K1019.M
Extraction Date :	11/15/2021	11/15/2021
Analysis Date :	11/18/2021	11/18/2021
Instrument :	KYLO	KYLO
Run :	1019K439	1019K440
Initials :	LSI	

Form 5  
Tune Summary

Lab Name: APPL Inc.  
Case No: \_\_\_\_\_  
Matrix: Water  
ID: 1019K001.D

SDG No: \_\_\_\_\_  
Date Analyzed: 10/19/2021  
Instrument: KYLO  
Time Analyzed: 13:58

Client Sample No.	APPL ID.	File ID.	Date Analyzed
1	0.1 ug/ml 10/10/21	1019K002.D	10/19/2021 14:09
2	0.2 ug/ml 10/10/21	1019K003.D	10/19/2021 14:29
3	0.5 ug/ml 10/10/21	1019K004.D	10/19/2021 14:49
4	1 ug/ml 10/10/21	1019K005.D	10/19/2021 15:09
5	5 ug/ml 10/10/21	1019K006.D	10/19/2021 15:29
6	10 ug/ml 10/10/21	1019K007.D	10/19/2021 15:49
7	50 ug/ml 10/10/21	1019K008.D	10/19/2021 16:09
8	100 ug/ml 10/10/21	1019K009.D	10/19/2021 16:29
9	SS ug/ml 10/10/21	1019K010.D	10/19/2021 16:49
10			
11			
12			
13			
14			
15			
16			
17			
18			
19			
20			
21			
22			

m/e

51 9.95 - 80.1% of mass 198	<u>36.8</u>
68 0 - 2.05% of mass 69	<u>1.7</u>
70 0 - 2% of mass 69	<u>0.4</u>
127 10 - 80% of mass 198	<u>54.6</u>
197 0 - 2% of mass 198	<u>0.2</u>
198 100 - 100% of mass 198	<u>100.0</u>
199 5 - 9% of mass 198	<u>6.5</u>
275 10 - 60% of mass 198	<u>23.2</u>
365 1 - 100% of mass 198	<u>2.5</u>
441 0.01 - 24% of mass 442	<u>13.9</u>
442 50 - 500% of mass 198	<u>73.4</u>
443 15 - 24% of mass 442	<u>18.4</u>

Form 5  
Tune Summary

Lab Name: APPL Inc.  
Case No: 98212  
Matrix: Water  
ID: 1019K436.D

SDG No: 98212  
Date Analyzed: 11/18/2021  
Instrument: KYLO  
Time Analyzed: 8:49

Client Sample No.	APPL ID.	File ID.	Date Analyzed	
1		5 ug/ml 10/19/21 (1)	1019K437.D	11/18/2021 9:01
2	Blank	211115A BLK 1/1000	1019K438.D	11/18/2021 9:21
3	Lab Control Spike	211115A LCS-1 1/1000	1019K439.D	11/18/2021 9:40
4	Lab Control SpikeD	211115A LCSD-1 1/100	1019K440.D	11/18/2021 10:00
5	ERH1907	BA46115W07 1/1000	1019K448.D	11/18/2021 12:40
6	ERH1909	BA46116W05 1/1000	1019K449.D	11/18/2021 13:00
7	ERH1915	BA46117W02 1/1010	1019K450.D	11/18/2021 13:20
8		5 ug/ml 10/13/21 (2)	1019K472.D	11/18/2021 20:38
9				
10				
11				
12				
13				
14				
15				
16				
17				
18				
19				
20				
21				
22				

m/e

51 9.95 - 80.1% of mass 198	<u>32.3</u>
68 0 - 2.05% of mass 69	<u>1.5</u>
70 0 - 2% of mass 69	<u>0.5</u>
127 10 - 80% of mass 198	<u>52.8</u>
197 0 - 2% of mass 198	<u>0.3</u>
198 100 - 100% of mass 198	<u>100.0</u>
199 5 - 9% of mass 198	<u>6.7</u>
275 10 - 60% of mass 198	<u>23.0</u>
365 1 - 100% of mass 198	<u>2.4</u>
441 0.01 - 24% of mass 442	<u>13.9</u>
442 50 - 500% of mass 198	<u>75.4</u>
443 15 - 24% of mass 442	<u>18.2</u>

8A  
INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: APPL Inc. Contract: \_\_\_\_\_  
 Lab Code: \_\_\_\_\_ SDG No.: \_\_\_\_\_  
 Lab File ID (Standard): 1019K437.D Date Analyzed: 11/18/21  
 Instrument ID: KYLO Time Analyzed: 9:01  
 GC Column: \_\_\_\_\_ ID: \_\_\_\_\_ Heated Purge: (Y/N) \_\_\_\_\_

		Napthalene-D8(IS)		Acenaphthene-D10(IS)		Phenanthrene-D10(IS)	
		AREA #	RT #	AREA #	RT #	AREA #	RT #
	12 HOUR STD	12784	3.86	6153	5.80	9197	7.49
	UPPER LIMIT	25568	4.03	12306	5.97	18394	7.66
	LOWER LIMIT	6392	3.69	3077	5.63	4599	7.32
	SAMPLE NO.						
01	211115A BLK 1/1000	12866	3.86	6185	5.79	9328	7.49
02	211115A LCS-1 1/1000	12352	3.86	6114	5.79	9269	7.49
03	211115A LCSD-1 1/1000	12851	3.86	6340	5.79	9491	7.49
04	BA46115W07 1/1000	14338	3.86	7099	5.79	10844	7.49
05	BA46116W05 1/1000	14604	3.86	7118	5.79	11034	7.49
06	BA46117W02 1/1010	14178	3.86	7028	5.79	10661	7.49
07	5 ug/ml 10/13/21 (2)	14852	3.86	7503	5.79	11571	7.49
08							
09							
10							
11							
12							
13							
14							
15							
16							
17							
18							
19							
20							
21							
22							

AREA UPPER LIMIT = +100% of internal standard area.  
 AREA LOWER LIMIT = -50% of internal standard area.  
 RT UPPER LIMIT = +0.17 minutes of internal standard RT  
 RT LOWER LIMIT = -0.17 minutes of internal standard RT

# Column used to flag values outside QC limits with an asterisk.  
 \* Values outside of QC limits.

8A  
INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: APPL Inc. Contract: \_\_\_\_\_  
 Lab Code: \_\_\_\_\_ SDG No.: \_\_\_\_\_  
 Lab File ID (Standard): 1019K437.D Date Analyzed: 11/18/21  
 Instrument ID: KYLO Time Analyzed: 9:01  
 GC Column: \_\_\_\_\_ ID: \_\_\_\_\_ Heated Purge: (Y/N) \_\_\_\_\_

	Chrysene-D12(IS)		Perylene-D12(IS)		AREA #	RT #
	AREA #	RT #	AREA #	RT #		
12 HOUR STD	11234	10.54	10043	12.71		
UPPER LIMIT	22468	10.71	20086	12.88		
LOWER LIMIT	5617	10.37	5022	12.54		
SAMPLE NO.						
01	211115A BLK 1/1000	11283	10.55	10568	12.71	
02	211115A LCS-1 1/1000	11195	10.54	10472	12.71	
03	211115A LCSD-1 1/1000	11677	10.54	10742	12.71	
04	BA46115W07 1/1000	13002	10.54	11849	12.71	
05	BA46116W05 1/1000	13219	10.54	12131	12.71	
06	BA46117W02 1/1010	12843	10.54	11559	12.71	
07	5 ug/ml 10/13/21 (2)	14376	10.54	13027	12.71	
08						
09						
10						
11						
12						
13						
14						
15						
16						
17						
18						
19						
20						
21						
22						

AREA UPPER LIMIT = +100% of internal standard area.  
 AREA LOWER LIMIT = -50% of internal standard area.  
 RT UPPER LIMIT = +0.17 minutes of internal standard RT  
 RT LOWER LIMIT = -0.17 minutes of internal standard RT

# Column used to flag values outside QC limits with an asterisk.  
 \* Values outside of QC limits.

# **EPA 8260B**

Form 2 & 8

## **Surrogate Recovery**

Lab Name: APPL, Inc.  
Case No: 98212  
Matrix: WATER

SDG No: 98212  
Date Analyzed: 11/19/2021  
Instrument: Thor

APPL ID.	Client Sample No.	SURROGATE: 1,2-DICHLOROETHANE-D4 (S)			SURROGATE: 4-BROMOFLUOROBENZENE (S)		
		Limits	Result	Qualifier	Limits	Result	Qualifier
211119BT-LCS	Lab Control Spike	81-118	112		85-114	108	
211119BT-LCSD	Lab Control SpikeD	81-118	114		85-114	106	
211119BT-BLK	Blank	81-118	116		85-114	102	
BA46117	ERH1915	81-118	114		85-114	102	

Comments: Batch: #86BTO-211119BT

Printed: 11/22/2021 1:07:45 PM  
Form 2 & 8, Surrogate Recovery Summary



# EPA 8260B

Form 2 & 8

## Surrogate Recovery

Lab Name: APPL, Inc.  
Case No: 98212  
Matrix: WATER

SDG No: 98212  
Date Analyzed: 11/19/2021  
Instrument: Thor

APPL ID.	Client Sample No.	SURROGATE: DIBROMOFLUOROMETHANE (S)			SURROGATE: TOLUENE-D8 (S)		
		Limits	Result	Qualifier	Limits	Result	Qualifier
211119BT-LCS	Lab Control Spike	80-119	115		89-112	105	
211119BT-LCSD	Lab Control SpikeD	80-119	114		89-112	102	
211119BT-BLK	Blank	80-119	113		89-112	103	
BA46117	ERH1915	80-119	116		89-112	103	

Comments: Batch: #86BTO-211119BT

Printed: 11/22/2021 1:07:45 PM  
Form 2 & 8, Surrogate Recovery Summary

# EPA 8260B

Form 2 & 8

## Surrogate Recovery

Lab Name: APPL, Inc.

SDG No: 98212

Case No: 98212

Date Analyzed: 11/15/2021

Matrix: WATER

Instrument: Max

APPL ID.	Client Sample No.	SURROGATE: 1,2-DICHLOROETHANE-D4 (S)			SURROGATE: 4-BROMOFLUOROBENZENE (S)		
		Limits	Result	Qualifier	Limits	Result	Qualifier
AM211115-LCS	Lab Control Spike	81-118	98.8		85-114	97.6	
AM211115-LCSD	Lab Control SpikeD	81-118	98.0		85-114	99.6	
AM211115-BLK	Blank	81-118	97.8		85-114	99.3	
BA46114	ERH1906	81-118	104		85-114	101	
BA46115	ERH1907	81-118	104		85-114	98.8	
BA46116	ERH1909	81-118	104		85-114	95.3	

Comments: Batch: #86BTO-AM211115

Printed: 11/22/2021 1:07:45 PM  
Form 2 & 8, Surrogate Recovery Summary

# EPA 8260B

Form 2 & 8

## Surrogate Recovery

Lab Name: APPL, Inc.  
Case No: 98212  
Matrix: WATER

SDG No: 98212  
Date Analyzed: 11/15/2021  
Instrument: Max

APPL ID.	Client Sample No.	SURROGATE: DIBROMOFLUOROMETHANE (S)			SURROGATE: TOLUENE-D8 (S)		
		Limits	Result	Qualifier	Limits	Result	Qualifier
AM211115-LCS	Lab Control Spike	80-119	99.2		89-112	97.6	
AM211115-LCSD	Lab Control SpikeD	80-119	99.2		89-112	99.2	
AM211115-BLK	Blank	80-119	102		89-112	97.7	
BA46114	ERH1906	80-119	106		89-112	98.1	
BA46115	ERH1907	80-119	107		89-112	99.5	
BA46116	ERH1909	80-119	107		89-112	94.4	

Comments: Batch: #86BTO-AM211115

Printed: 11/22/2021 1:07:45 PM  
Form 2 & 8, Surrogate Recovery Summary

# **EPA 8260B**

Form 4

## **Blank Summary**

Lab Name: APPL, Inc.  
Case No: 98212  
Matrix: WATER  
Blank ID: 211119BT-BLK

SDG No: 98212  
Date Analyzed: 11/20/2021  
Instrument: Thor  
Time Analyzed: 0039

<b>APPL ID.</b>	<b>Client Sample No.</b>	<b>File ID.</b>	<b>Date Analyzed</b>
211119BT-LCS	Lab Control Spike	1119T31	11/19/2021 2211
211119BT-LCSD	Lab Control Spiked	1119T32	11/19/2021 2236
211119BT-BLK	Blank	1119T37	11/20/2021 0039
BA46117	ERH1915	1119T38	11/20/2021 0103

Comments: Batch: #86BTO-211119BT

Printed: 11/22/2021 1:07:14 PM  
Form 4, Blank Summary

# EPA 8260B

Form 4

## Blank Summary

Lab Name: APPL, Inc.

SDG No: 98212

Case No: 98212

Date Analyzed: 11/15/2021

Matrix: WATER

Instrument: Max

Blank ID: AM211115-BLK

Time Analyzed: 1150

<b>APPL ID.</b>	<b>Client Sample No.</b>	<b>File ID.</b>	<b>Date Analyzed</b>
AM211115-LCS	Lab Control Spike	1115M03	11/15/2021 0928
AM211115-LCSD	Lab Control Spiked	1115M04	11/15/2021 0957
AM211115-BLK	Blank	1115M08	11/15/2021 1150
BA46114	ERH1906	1115M12	11/15/2021 1344
BA46115	ERH1907	1115M13	11/15/2021 1412
BA46116	ERH1909	1115M14	11/15/2021 1440

Comments: Batch: #86BTO-AM211115

Printed: 11/22/2021 1:07:14 PM  
Form 4, Blank Summary

**Method Blank**  
**EPA 8260B BTEX WATER**

Blank Name/QCG: **AM2111W-46000 - 270528**  
Batch ID: #86BTO-AM211115

APPL Inc.  
908 North Temperance Avenue  
Clovis, CA 93611

Sample Type	Analyte	Result	LOQ	LOD	DL	Units	Extraction Date	Analysis Date
BLANK	BENZENE	0.30 U	1.0	0.30	0.15	ug/L	11/15/2021	11/15/2021
BLANK	ETHYLBENZENE	0.50 U	1.0	0.50	0.23	ug/L	11/15/2021	11/15/2021
BLANK	TOLUENE	0.30 U	1.0	0.30	0.15	ug/L	11/15/2021	11/15/2021
BLANK	XYLENES (TOTAL)	0.30 U	2.0	0.30	0.15	ug/L	11/15/2021	11/15/2021
BLANK	SURROGATE: 1,2-DICHLOROET	97.8	81-118			%	11/15/2021	11/15/2021
BLANK	SURROGATE: 4-BROMOFLUORO	99.3	85-114			%	11/15/2021	11/15/2021
BLANK	SURROGATE: DIBROMOFLUOR	102	80-119			%	11/15/2021	11/15/2021
BLANK	SURROGATE: TOLUENE-D8 (S)	97.7	89-112			%	11/15/2021	11/15/2021

Quant Method:M1111W.M  
Run #:1115M08  
Instrument:Max  
Sequence:211111  
Initials: PAN

GC SC-Blank-REG MDLs-DOD  
Printed: 11/22/2021 1:09:06 PM

**Method Blank**  
**EPA 8260B BTEX WATER**

Blank Name/QCG: **211119W-46117 - 270806**  
Batch ID: #86BTO-211119BT

APPL Inc.  
908 North Temperance Avenue  
Clovis, CA 93611

Sample Type	Analyte	Result	LOQ	LOD	DL	Units	Extraction Date	Analysis Date
BLANK	BENZENE	0.30 U	1.0	0.30	0.15	ug/L	11/20/2021	11/20/2021
BLANK	ETHYLBENZENE	0.50 U	1.0	0.50	0.23	ug/L	11/20/2021	11/20/2021
BLANK	TOLUENE	0.30 U	1.0	0.30	0.15	ug/L	11/20/2021	11/20/2021
BLANK	XYLENES (TOTAL)	0.30 U	2.0	0.30	0.15	ug/L	11/20/2021	11/20/2021
BLANK	SURROGATE: 1,2-DICHLOROET	116	81-118			%	11/20/2021	11/20/2021
BLANK	SURROGATE: 4-BROMOFLUORO	102	85-114			%	11/20/2021	11/20/2021
BLANK	SURROGATE: DIBROMOFLUOR	113	80-119			%	11/20/2021	11/20/2021
BLANK	SURROGATE: TOLUENE-D8 (S)	103	89-112			%	11/20/2021	11/20/2021

Quant Method: T1109W.M  
Run #: 1119T37  
Instrument: Thor  
Sequence: 211111  
Initials: EOG

GC SC-Blank-REG MDLs-DOD  
Printed: 11/22/2021 1:09:06 PM

# EPA 8260B

Form 4

## LCS Summary

Lab Name: APPL, Inc.  
Case No: 98212  
Matrix: WATER  
LCS ID: 211119BT-LCS

SDG No: 98212  
Date Analyzed: 11/19/2021  
Instrument: Thor  
Time Analyzed: 2211

<b>APPL ID.</b>	<b>Client Sample No.</b>	<b>File ID.</b>	<b>Date Analyzed</b>
211119BT-LCS	Lab Control Spike	1119T31	11/19/2021 2211
211119BT-LCSD	Lab Control Spiked	1119T32	11/19/2021 2236
211119BT-BLK	Blank	1119T37	11/20/2021 0039
BA46117	ERH1915	1119T38	11/20/2021 0103

Comments: Batch: #86BTO-211119BT

Printed: 11/22/2021 1:06:54 PM  
Form 4, LCS Summary



# EPA 8260B

Form 4

## LCS Summary

Lab Name: APPL, Inc.  
Case No: 98212  
Matrix: WATER  
LCS ID: AM211115-LCS

SDG No: 98212  
Date Analyzed: 11/15/2021  
Instrument: Max  
Time Analyzed: 0928

<b>APPL ID.</b>	<b>Client Sample No.</b>	<b>File ID.</b>	<b>Date Analyzed</b>
AM211115-LCS	Lab Control Spike	1115M03	11/15/2021 0928
AM211115-LCSD	Lab Control Spiked	1115M04	11/15/2021 0957
AM211115-BLK	Blank	1115M08	11/15/2021 1150
BA46114	ERH1906	1115M12	11/15/2021 1344
BA46115	ERH1907	1115M13	11/15/2021 1412
BA46116	ERH1909	1115M14	11/15/2021 1440

Comments: Batch: #86BTO-AM211115

Printed: 11/22/2021 1:06:54 PM  
Form 4, LCS Summary

# Laboratory Control Spike Recoveries

## EPA 8260B BTEX WATER

APPL ID: 211115W-46000 LCS - 270528

Batch ID: #86BTO-AM211115

APPL Inc.

908 North Temperance Avenue

Clovis, CA 93611

Compound Name	Spike Lvl ug/L	SPK Result ug/L	DUP Result ug/L	SPK % Recovery	DUP % Recovery	Recovery Limits	RPD %	RPD Limits
BENZENE	10.00	10.4	9.64	104	96.4	79-120	7.6	20
ETHYLBENZENE	10.00	10.7	10.4	107	104	79-121	2.8	20
TOLUENE	10.00	10.3	9.37	103	93.7	80-121	9.5	20
XYLENES (TOTAL)	30.0	31.1	29.9	104	99.7	79-121	3.9	20
-----								
SURROGATE: 1,2-DICHLOROETHANE-D	25.0	24.7	24.5	98.8	98.0	81-118		
SURROGATE: 4-BROMOFLUOROBENZE	25.0	24.4	24.9	97.6	99.6	85-114		
SURROGATE: DIBROMOFLUOROMETH	25.0	24.8	24.8	99.2	99.2	80-119		
SURROGATE: TOLUENE-D8 (S)	25.0	24.4	24.8	97.6	99.2	89-112		
-----								

Comments: \_\_\_\_\_

<u>Primary</u>	<u>SPK</u>	<u>DUP</u>
Quant Method :	M1111W.M	M1111W.M
Extraction Date :	11/15/2021	11/15/2021
Analysis Date :	11/15/2021	11/15/2021
Instrument :	Max	Max
Run :	1115M03	1115M04
Initials :	PAN	

# Laboratory Control Spike Recoveries

## EPA 8260B BTEX WATER

APPL ID: 211119W-46117 LCS - 270806

Batch ID: #86BTO-211119BT

APPL Inc.

908 North Temperance Avenue

Clovis, CA 93611

Compound Name	Spike Lvl ug/L	SPK Result ug/L	DUP Result ug/L	SPK % Recovery	DUP % Recovery	Recovery Limits	RPD %	RPD Limits
BENZENE	10.00	8.98	9.16	89.8	91.6	79-120	2.0	20
ETHYLBENZENE	10.00	9.15	9.58	91.5	95.8	79-121	4.6	20
TOLUENE	10.00	9.51	9.70	95.1	97.0	80-121	2.0	20
XYLENES (TOTAL)	30.0	28.4	29.1	94.7	97.0	79-121	2.4	20
-----								
SURROGATE: 1,2-DICHLOROETHANE-D	25.0	28.1	28.4	112	114	81-118		
SURROGATE: 4-BROMOFLUOROBENZE	25.0	26.9	26.5	108	106	85-114		
SURROGATE: DIBROMOFLUOROMETH	25.0	28.7	28.6	115	114	80-119		
SURROGATE: TOLUENE-D8 (S)	25.0	26.2	25.6	105	102	89-112		
-----								

Comments: \_\_\_\_\_

<u>Primary</u>	<u>SPK</u>	<u>DUP</u>
Quant Method :	T1109W.M	T1109W.M
Extraction Date :	11/19/2021	11/19/2021
Analysis Date :	11/19/2021	11/19/2021
Instrument :	Thor	Thor
Run :	1119T31	1119T32
Initials :	EOG	

Form 5  
Tune Summary

Lab Name: APPL Inc.  
Case No: \_\_\_\_\_  
Matrix: Water  
ID: 1111M21.D

SDG No: \_\_\_\_\_  
Date Analyzed: 11/11/2021  
Instrument: Max  
Time Analyzed: 18:10

Client Sample No.	APPL ID.	File ID.	Date Analyzed
1	0.3ug/L VOC STD 11/1	1111M22.D	11/11/2021 18:38
2	0.5ug/L VOC STD 11/1	1111M23.D	11/11/2021 19:07
3	1ug/L VOC STD 11/11/	1111M24.D	11/11/2021 19:35
4	2ug/L VOC STD 11/11/	1111M25.D	11/11/2021 20:03
5	5ug/L VOC STD 11/11/	1111M26.D	11/11/2021 20:32
6	10ug/L VOC STD 11/11	1111M27.D	11/11/2021 21:00
7	20ug/L VOC STD 11/11	1111M28.D	11/11/2021 21:28
8	40ug/L VOC STD 11/11	1111M29.D	11/11/2021 21:57
9	100ug/L VOC STD 11/1	1111M30.D	11/11/2021 22:25
10	(SS) 10ug/L VOC STD	1111M32.D	11/11/2021 23:22
11			
12			
13			
14			
15			
16			
17			
18			
19			
20			
21			
22			

m/e

50 15 - 40% of mass 95	<u>20.6</u>
75 30 - 60.04% of mass 95	<u>56.9</u>
95 100 - 200% of mass 95	<u>100.0</u>
96 5 - 9% of mass 95	<u>6.4</u>
173 0 - 2% of mass 174	<u>0.0</u>
174 50 - 200% of mass 95	<u>123.3</u>
175 5 - 9.02% of mass 174	<u>8.8</u>
176 95 - 101% of mass 174	<u>100.5</u>
177 5 - 9% of mass 176	<u>7.0</u>

8A  
INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: APPL Inc. Contract: \_\_\_\_\_  
 Lab Code: \_\_\_\_\_ SDG No.: \_\_\_\_\_  
 Lab File ID (Standard): 1111M27.D Date Analyzed: 11/11/21  
 Instrument ID: Max Time Analyzed: 21:00  
 GC Column: \_\_\_\_\_ ID: \_\_\_\_\_ Heated Purge: (Y/N) \_\_\_\_\_

	Fluorobenzene (IS)		Chlorobenzene-D5 (IS)		1,4-Dichlorobenzene-D (IS)	
	AREA #	RT #	AREA #	RT #	AREA #	RT #
12 HOUR STD	400946	6.37	356817	9.53	231463	11.85
UPPER LIMIT	801892	6.54	713634	9.70	462926	12.02
LOWER LIMIT	200473	6.20	178409	9.36	115732	11.68
SAMPLE NO.						
01 0.3ug/L VOC STD 11/11/21	412529	6.37	369810	9.53	213533	11.85
02 0.5ug/L VOC STD 11/11/21	412615	6.37	365084	9.53	207406	11.85
03 1ug/L VOC STD 11/11/21	406373	6.37	352913	9.53	215896	11.85
04 2ug/L VOC STD 11/11/21	404400	6.37	350989	9.53	214879	11.85
05 5ug/L VOC STD 11/11/21	411540	6.37	360431	9.53	229293	11.85
06 10ug/L VOC STD 11/11/21	400946	6.37	356817	9.53	231463	11.85
07 20ug/L VOC STD 11/11/21	404029	6.37	358338	9.53	243425	11.85
08 40ug/L VOC STD 11/11/21	410532	6.37	372777	9.53	245394	11.84
09 100ug/L VOC STD 11/11/21	401409	6.37	366234	9.53	257008	11.84
10 (SS) 10ug/L VOC STD 11/11/21	431765	6.37	384615	9.52	244603	11.84
11						
12						
13						
14						
15						
16						
17						
18						
19						
20						
21						
22						

AREA UPPER LIMIT = +100% of internal standard area.  
 AREA LOWER LIMIT = -50% of internal standard area.  
 RT UPPER LIMIT = +0.17 minutes of internal standard RT  
 RT LOWER LIMIT = -0.17 minutes of internal standard RT

# Column used to flag values outside QC limits with an asterisk.  
 \* Values outside of QC limits.

Form 5  
Tune Summary

Lab Name: APPL Inc.  
 Case No: \_\_\_\_\_  
 Matrix: Water  
 ID: 1109T13.D

SDG No: \_\_\_\_\_  
 Date Analyzed: 11/9/2021  
 Instrument: Thor  
 Time Analyzed: 11:23

Client Sample No.	APPL ID.	File ID.	Date Analyzed
1	0.3ug/L VOC STD 11/9	1109T14.D	11/9/2021 11:48
2	0.5ug/L VOC STD 11/9	1109T15.D	11/9/2021 12:13
3	1ug/L VOC STD 11/9/2	1109T16.D	11/9/2021 12:38
4	2ug/L VOC STD 11/9/2	1109T17.D	11/9/2021 13:03
5	5ug/L VOC STD 11/9/2	1109T18.D	11/9/2021 13:28
6	10ug/L VOC STD 11/9/	1109T19.D	11/9/2021 13:52
7	20ug/L VOC STD 11/9/	1109T20.D	11/9/2021 14:17
8	40ug/L VOC STD 11/9/	1109T21.D	11/9/2021 14:42
9	100ug/L VOC STD 11/9	1109T22.D	11/9/2021 15:07
10	(SS) 10ug/L VOC STD	1109T24.D	11/9/2021 15:57
11			
12			
13			
14			
15			
16			
17			
18			
19			
20			
21			
22			

m/e

50 15 - 40% of mass 95	<u>16.1</u>
75 30 - 60% of mass 95	<u>50.2</u>
95 100 - 100% of mass 95	<u>100.0</u>
96 5 - 9% of mass 95	<u>6.4</u>
173 0 - 2.3% of mass 174	<u>0.0</u>
174 50 - 200% of mass 95	<u>145.6</u>
175 5 - 9% of mass 174	<u>8.1</u>
176 95 - 101% of mass 174	<u>99.8</u>
177 5 - 9% of mass 176	<u>6.1</u>

8A  
INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: APPL Inc. Contract: \_\_\_\_\_  
 Lab Code: \_\_\_\_\_ SDG No.: \_\_\_\_\_  
 Lab File ID (Standard): 1109T19.D Date Analyzed: 9 Nov 21 13:52  
 Instrument ID: Thor Time Analyzed: 9 Nov 21 13:52  
 GC Column: \_\_\_\_\_ ID: \_\_\_\_\_ Heated Purge: (Y/N) \_\_\_\_\_

	Fluorobenzene (IS)		Chlorobenzene-D5 (IS)		1,4-Dichlorobenzene-D (IS)		
	AREA #	RT #	AREA #	RT #	AREA #	RT #	
12 HOUR STD	316124	6.35	306509	9.81	216025	12.37	
UPPER LIMIT	632248	6.52	613018	9.98	432050	12.54	
LOWER LIMIT	158062	6.18	153255	9.64	108013	12.20	
SAMPLE NO.							
01	0.3ug/L VOC STD 11/9/21	320118	6.35	309209	9.81	205673	12.37
02	0.5ug/L VOC STD 11/9/21	311081	6.35	300686	9.81	205596	12.37
03	1ug/L VOC STD 11/9/21	315410	6.35	306467	9.81	215832	12.37
04	2ug/L VOC STD 11/9/21	310022	6.35	303468	9.81	213648	12.37
05	5ug/L VOC STD 11/9/21	308169	6.35	300381	9.81	211820	12.37
06	10ug/L VOC STD 11/9/21	316124	6.35	306509	9.81	216025	12.37
07	20ug/L VOC STD 11/9/21	311782	6.34	308423	9.81	212717	12.37
08	40ug/L VOC STD 11/9/21	306148	6.34	296587	9.81	207105	12.37
09	100ug/L VOC STD 11/9/21	311870	6.34	300158	9.81	206230	12.37
10	(SS) 10ug/L VOC STD 11/9/21	310765	6.34	306633	9.81	215446	12.37
11							
12							
13							
14							
15							
16							
17							
18							
19							
20							
21							
22							

AREA UPPER LIMIT = +100% of internal standard area.  
 AREA LOWER LIMIT = -50% of internal standard area.  
 RT UPPER LIMIT = +0.17 minutes of internal standard RT  
 RT LOWER LIMIT = -0.17 minutes of internal standard RT

# Column used to flag values outside QC limits with an asterisk.  
 \* Values outside of QC limits.

Form 5  
Tune Summary

Lab Name: APPL Inc.  
 Case No: 98212  
 Matrix: Water  
 ID: 1115M01.D

SDG No: 98212  
 Date Analyzed: 11/15/2021  
 Instrument: Max  
 Time Analyzed: 8:32

	Client Sample No.	APPL ID.	File ID.	Date Analyzed
1	Lab Control Spike	211115A CCV/LCS 10ug	1115M03.D	11/15/2021 9:28
2	Lab Control SpikeD	211115A LCSD 10ug/L	1115M04.D	11/15/2021 9:57
3	Blank	211115A BLK	1115M08.D	11/15/2021 11:50
4	ERH1906	BA46114W01	1115M12.D	11/15/2021 13:44
5	ERH1907	BA46115W01	1115M13.D	11/15/2021 14:12
6	ERH1909	BA46116W01	1115M14.D	11/15/2021 14:40
7		Ending CCV 10ug/L 11	1115M25.D	11/15/2021 19:52
8				
9				
10				
11				
12				
13				
14				
15				
16				
17				
18				
19				
20				
21				
22				

m/e

50 15 - 40% of mass 95	<u>19.0</u>
75 30 - 60.04% of mass 95	<u>59.5</u>
95 100 - 200% of mass 95	<u>100.0</u>
96 5 - 9% of mass 95	<u>6.7</u>
173 0 - 2% of mass 174	<u>0.0</u>
174 50 - 200% of mass 95	<u>126.9</u>
175 5 - 9.02% of mass 174	<u>7.8</u>
176 95 - 101% of mass 174	<u>100.5</u>
177 5 - 9% of mass 176	<u>6.9</u>



8A  
INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: APPL Inc. Contract: \_\_\_\_\_  
 Lab Code: \_\_\_\_\_ SDG No.: \_\_\_\_\_  
 Lab File ID (Standard): 1115M03.D Date Analyzed: 11/15/21  
 Instrument ID: Max Time Analyzed: 9:28  
 GC Column: \_\_\_\_\_ ID: \_\_\_\_\_ Heated Purge: (Y/N) \_\_\_\_\_

	Fluorobenzene (IS)		Chlorobenzene-D5 (IS)		1,4-Dichlorobenzene-D (IS)		
	AREA #	RT #	AREA #	RT #	AREA #	RT #	
12 HOUR STD	414024	6.38	371836	9.53	236811	11.85	
UPPER LIMIT	828048	6.55	743672	9.70	473622	12.02	
LOWER LIMIT	207012	6.21	185918	9.36	118406	11.68	
SAMPLE NO.							
01	211115A CCV/LCS 10ug	414024	6.38	371836	9.53	236811	11.85
02	211115A LCSD 10ug/L	411326	6.38	355924	9.53	229762	11.85
03	211115A BLK	395694	6.38	350184	9.53	211146	11.85
04	BA46114W01	363931	6.38	329377	9.53	206728	11.85
05	BA46115W01	382634	6.38	339368	9.53	200988	11.85
06	BA46116W01	376769	6.38	341407	9.53	199848	11.85
07	Ending CCV 10ug/L 11/	380344	6.37	342457	9.53	222128	11.85
08							
09							
10							
11							
12							
13							
14							
15							
16							
17							
18							
19							
20							
21							
22							

AREA UPPER LIMIT = +100% of internal standard area.  
 AREA LOWER LIMIT = -50% of internal standard area.  
 RT UPPER LIMIT = +0.17 minutes of internal standard RT  
 RT LOWER LIMIT = -0.17 minutes of internal standard RT

# Column used to flag values outside QC limits with an asterisk.  
 \* Values outside of QC limits.

Form 5  
Tune Summary

Lab Name: APPL Inc.  
 Case No: 98212  
 Matrix: Water  
 ID: 1119T30.D

SDG No: 98212  
 Date Analyzed: 11/19/2021  
 Instrument: Thor  
 Time Analyzed: 21:46

	Client Sample No.	APPL ID.	File ID.	Date Analyzed
1	Lab Control Spike	211119B CCV/LCS 10ug	1119T31.D	11/19/2021 22:11
2	Lab Control SpikeD	211119B LCSD 10ug/L	1119T32.D	11/19/2021 22:36
3	Blank	211119B BLK	1119T37.D	11/20/2021 0:39
4	ERH1915	BA46117W07	1119T38.D	11/20/2021 1:03
5		Ending CCV 10ug/L 11	1119T52.D	11/20/2021 6:47
6				
7				
8				
9				
10				
11				
12				
13				
14				
15				
16				
17				
18				
19				
20				
21				
22				

m/e

50 15 - 40% of mass 95	<u>16.0</u>
75 30 - 60% of mass 95	<u>52.5</u>
95 100 - 100% of mass 95	<u>100.0</u>
96 5 - 9% of mass 95	<u>6.7</u>
173 0 - 2.3% of mass 174	<u>0.0</u>
174 50 - 200% of mass 95	<u>166.4</u>
175 5 - 9% of mass 174	<u>7.7</u>
176 95 - 101% of mass 174	<u>98.2</u>
177 5 - 9% of mass 176	<u>6.5</u>

8A  
INTERNAL STANDARD AREA AND RT SUMMARY

Lab Name: APPL Inc. Contract: \_\_\_\_\_  
 Lab Code: \_\_\_\_\_ SDG No.: \_\_\_\_\_  
 Lab File ID (Standard): 1119T31.D Date Analyzed: 11/19/21  
 Instrument ID: Thor Time Analyzed: 22:11  
 GC Column: \_\_\_\_\_ ID: \_\_\_\_\_ Heated Purge: (Y/N) \_\_\_\_\_

	Fluorobenzene (IS)		Chlorobenzene-D5 (IS)		1,4-Dichlorobenzene-D (IS)		
	AREA #	RT #	AREA #	RT #	AREA #	RT #	
12 HOUR STD	251289	6.35	252734	9.81	190553	12.37	
UPPER LIMIT	502578	6.52	505468	9.98	381106	12.54	
LOWER LIMIT	125645	6.18	126367	9.64	95277	12.20	
SAMPLE NO.							
01	211119B CCV/LCS 10ug	251289	6.35	252734	9.81	190553	12.37
02	211119B LCSD 10ug/L	256465	6.34	260381	9.81	196706	12.37
03	211119B BLK	253564	6.35	256153	9.81	187736	12.37
04	BA46117W07	253667	6.34	256675	9.81	186147	12.37
05	Ending CCV 10ug/L 11/	252617	6.34	260147	9.81	196942	12.37
06							
07							
08							
09							
10							
11							
12							
13							
14							
15							
16							
17							
18							
19							
20							
21							
22							

AREA UPPER LIMIT = +100% of internal standard area.  
 AREA LOWER LIMIT = -50% of internal standard area.  
 RT UPPER LIMIT = +0.17 minutes of internal standard RT  
 RT LOWER LIMIT = -0.17 minutes of internal standard RT

# Column used to flag values outside QC limits with an asterisk.  
 \* Values outside of QC limits.

# EPA 8260B

Form 2 & 8

## Surrogate Recovery

Lab Name: APPL, Inc.  
Case No: 98212  
Matrix: WATER

SDG No: 98212  
Date Analyzed: 11/15/2021  
Instrument: Max

APPL ID.	Client Sample No.	SURROGATE: 4-BROMOFLUOROBENZENE (S)			Limits	Result	Qualifier
		Limits	Result	Qualifier			
211115AM-LCS	Lab Control Spike	85-114	98.0				
211115AM-LCSD	Lab Control SpikeD	85-114	97.6				
211115AM-BLK	Blank	85-114	98.4				
BA46114	ERH1906	85-114	100.0				
BA46115	ERH1907	85-114	97.8				
BA46116	ERH1909	85-114	94.4				

Comments: Batch: #GRO86-211115AM

Printed: 11/23/2021 9:04:54 AM  
Form 2 & 8, Surrogate Recovery Summary

# EPA 8260B

Form 2 & 8

## Surrogate Recovery

Lab Name: APPL, Inc.  
Case No: 98212  
Matrix: WATER

SDG No: 98212  
Date Analyzed: 11/19/2021  
Instrument: Thor

APPL ID.	Client Sample No.	SURROGATE: 4-BROMOFLUOROBENZENE (S)			Limits	Result	Qualifier
		Limits	Result	Qualifier			
211119BT-LCS	Lab Control Spike	85-114	104				
211119BT-LCSD	Lab Control SpikeD	85-114	106				
211119BT-BLK	Blank	85-114	103				
BA46117	ERH1915	85-114	102				

Comments: Batch: #GRO86-211119BT

# **EPA 8260B**

Form 4

## **Blank Summary**

Lab Name: APPL, Inc.  
Case No: 98212  
Matrix: WATER  
Blank ID: 211115AM-BLK

SDG No: 98212  
Date Analyzed: 11/15/2021  
Instrument: Max  
Time Analyzed: 1150

<b>APPL ID.</b>	<b>Client Sample No.</b>	<b>File ID.</b>	<b>Date Analyzed</b>
211115AM-LCS	Lab Control Spike	1115M06	11/15/2021 1053
211115AM-LCSD	Lab Control Spiked	1115M07	11/15/2021 1122
211115AM-BLK	Blank	1115M08	11/15/2021 1150
BA46114	ERH1906	1115M12	11/15/2021 1344
BA46115	ERH1907	1115M13	11/15/2021 1412
BA46116	ERH1909	1115M14	11/15/2021 1440

Comments: Batch: #GRO86-211115AM

Printed: 11/23/2021 9:04:30 AM  
Form 4, Blank Summary

# EPA 8260B

Form 4

## Blank Summary

Lab Name: APPL, Inc.  
Case No: 98212  
Matrix: WATER  
Blank ID: 211119BT-BLK

SDG No: 98212  
Date Analyzed: 11/20/2021  
Instrument: Thor  
Time Analyzed: 0039

<b>APPL ID.</b>	<b>Client Sample No.</b>	<b>File ID.</b>	<b>Date Analyzed</b>
211119BT-LCS	Lab Control Spike	1119T35	11/19/2021 2349
211119BT-LCSD	Lab Control Spiked	1119T36	11/20/2021 0014
211119BT-BLK	Blank	1119T37	11/20/2021 0039
BA46117	ERH1915	1119T38	11/20/2021 0103

Comments: Batch: #GRO86-211119BT

Printed: 11/23/2021 9:04:30 AM  
Form 4, Blank Summary

**Method Blank**  
**EPA 8260B GRO WATER**

Blank Name/QCG: **211119W-46117 - 270816**  
Batch ID: #GRO86-211119BT

APPL Inc.  
908 North Temperance Avenue  
Clovis, CA 93611

Sample Type	Analyte	Result	LOQ	LOD	DL	Units	Extraction Date	Analysis Date
BLANK	GASOLINE RANGE ORGANICS	18.0 U	20	18.0	8.6	ug/L	11/20/2021	11/20/2021
BLANK	SURROGATE: 4-BROMOFLUORO	103	85-114			%	11/20/2021	11/20/2021

Quant Method: TGAS1015.M  
Run #: 1119T37  
Instrument: Thor  
Sequence: 211111  
Initials: EOG

GC SC-Blank-REG MDLs-DOD  
Printed: 11/23/2021 9:06:01 AM



**Method Blank**  
**EPA 8260B GRO WATER**

Blank Name/QCG: **211115W-46000 - 270843**  
Batch ID: #GRO86-211115AM

APPL Inc.  
908 North Temperance Avenue  
Clovis, CA 93611

Sample Type	Analyte	Result	LOQ	LOD	DL	Units	Extraction Date	Analysis Date
BLANK	GASOLINE RANGE ORGANICS	18.0 U	20	18.0	8.6	ug/L	11/15/2021	11/15/2021
BLANK	SURROGATE: 4-BROMOFLUORO	98.4	85-114			%	11/15/2021	11/15/2021

Quant Method:MGAS0825.M  
Run #:1115M08  
Instrument:Max  
Sequence:211111  
Initials: PAN

GC SC-Blank-REG MDLs-DOD  
Printed: 11/23/2021 9:06:01 AM

# EPA 8260B

Form 4

## LCS Summary

Lab Name: APPL, Inc.  
Case No: 98212  
Matrix: WATER  
LCS ID: 211115AM-LCS

SDG No: 98212  
Date Analyzed: 11/15/2021  
Instrument: Max  
Time Analyzed: 1053

<b>APPL ID.</b>	<b>Client Sample No.</b>	<b>File ID.</b>	<b>Date Analyzed</b>
211115AM-LCS	Lab Control Spike	1115M06	11/15/2021 1053
211115AM-LCSD	Lab Control Spiked	1115M07	11/15/2021 1122
211115AM-BLK	Blank	1115M08	11/15/2021 1150
BA46114	ERH1906	1115M12	11/15/2021 1344
BA46115	ERH1907	1115M13	11/15/2021 1412
BA46116	ERH1909	1115M14	11/15/2021 1440

Comments: Batch: #GRO86-211115AM

Printed: 11/23/2021 8:58:54 AM  
Form 4, LCS Summary

# EPA 8260B

Form 4

## LCS Summary

Lab Name: APPL, Inc.

SDG No: 98212

Case No: 98212

Date Analyzed: 11/19/2021

Matrix: WATER

Instrument: Thor

LCS ID: 211119BT-LCS

Time Analyzed: 2349

<b>APPL ID.</b>	<b>Client Sample No.</b>	<b>File ID.</b>	<b>Date Analyzed</b>
211119BT-LCS	Lab Control Spike	1119T35	11/19/2021 2349
211119BT-LCSD	Lab Control Spiked	1119T36	11/20/2021 0014
211119BT-BLK	Blank	1119T37	11/20/2021 0039
BA46117	ERH1915	1119T38	11/20/2021 0103

Comments: Batch: #GRO86-211119BT

Printed: 11/23/2021 8:58:54 AM  
Form 4, LCS Summary

# Laboratory Control Spike Recoveries

## EPA 8260B GRO WATER

APPL ID: 211115W-46000 LCS - 270843

Batch ID: #GRO86-211115AM

APPL Inc.

908 North Temperance Avenue

Clovis, CA 93611

Compound Name	Spike Lvl ug/L	SPK Result ug/L	DUP Result ug/L	SPK % Recovery	DUP % Recovery	Recovery Limits	RPD %	RPD Limits
GASOLINE RANGE ORGANICS	300	327	332	109	111	78-122	1.5	20
SURROGATE: 4-BROMOFLUOROBENZE	25.0	24.5	24.4	98.0	97.6	85-114		

Comments: \_\_\_\_\_

<u>Primary</u>	<u>SPK</u>	<u>DUP</u>
Quant Method :	MGAS0825.M	MGAS0825.M
Extraction Date :	11/15/2021	11/15/2021
Analysis Date :	11/15/2021	11/15/2021
Instrument :	Max	Max
Run :	1115M06	1115M07
Initials :	PAN	

# Laboratory Control Spike Recoveries

## EPA 8260B GRO WATER

APPL ID: 211119W-46117 LCS - 270816  
 Batch ID: #GRO86-211119BT

APPL Inc.  
 908 North Temperance Avenue  
 Clovis, CA 93611

Compound Name	Spike Lvl ug/L	SPK Result ug/L	DUP Result ug/L	SPK % Recovery	DUP % Recovery	Recovery Limits	RPD %	RPD Limits
GASOLINE RANGE ORGANICS	300	302	306	101	102	78-122	1.3	20
SURROGATE: 4-BROMOFLUOROBENZE	25.0	26.0	26.5	104	106	85-114		

Comments: \_\_\_\_\_

<u>Primary</u>	<u>SPK</u>	<u>DUP</u>
Quant Method :	TGAS1015.M	TGAS1015.M
Extraction Date :	11/19/2021	11/20/2021
Analysis Date :	11/19/2021	11/20/2021
Instrument :	Thor	Thor
Run :	1119T35	1119T36
Initials :	EOG	

# **SW846 9060A**

Form 4

## **Blank Summary**

Lab Name: APPL, Inc.  
Case No: 98212  
Matrix: WATER  
Blank ID: 211119A-BLK

SDG No: 98212  
Date Analyzed: 11/19/2021  
Instrument: TICTOC  
Time Analyzed: 1308

<b>APPL ID.</b>	<b>Client Sample No.</b>	<b>File ID.</b>	<b>Date Analyzed</b>
211119A-LCS	Lab Control Spike	24	11/19/2021 1225
211119A-BLK	Blank	25	11/19/2021 1308
211119A-LCSD	Lab Control Spiked	27	11/19/2021 2046
BA46115	ERH1907	32	11/20/2021 0015
BA46117	ERH1915	33	11/20/2021 0057

Comments: Batch: #TOCW5-211119A

# WETLAB BLANK

APPL Inc.  
908 North Temperance Avenue  
Clovis, CA 93611

Method	Analyte	Result	LOQ	LOD	DL	Units	Prep Date	Analysis Date	QC Group
SW846 90	TOTAL ORGANIC C	0.350 U	0.93	0.350	0.130	mg/L	11/19/21	11/19/21	#TOCW5-211119A-BA45998

# **SW846 9060A**

Form 4

## **LCS Summary**

Lab Name: APPL, Inc.  
Case No: 98212  
Matrix: WATER  
LCS ID: 211119A-LCS

SDG No: 98212  
Date Analyzed: 11/19/2021  
Instrument: TICTOC  
Time Analyzed: 1225

<b>APPL ID.</b>	<b>Client Sample No.</b>	<b>File ID.</b>	<b>Date Analyzed</b>
211119A-LCS	Lab Control Spike	24	11/19/2021 1225
211119A-BLK	Blank	25	11/19/2021 1308
211119A-LCSD	Lab Control Spiked	27	11/19/2021 2046
BA46115	ERH1907	32	11/20/2021 0015
BA46117	ERH1915	33	11/20/2021 0057

Comments: Batch: #TOCW5-211119A



# Laboratory Control Spike Recoveries

## WETLAB

APPL Inc.  
908 North Temperance Avenue  
Clovis, CA 93611

Method	Compound Name	Spike Lvl mg/L	SPK Res mg/L	DUP Res mg/L	SPK % Recov	DUP % Recov	RPD	RPD Max	QC Limits	Extract Date-Spk	Analysis Date-Spk	Extract Date-Dup	Analysis Date-Dup	QC Group
SW846 90	TOTAL ORGANIC CARBO	5.00	4.32	4.28	86.4	85.6	0.93	20	80-120	11/19/21	11/19/21	11/19/21	11/19/21	#TOCW5-211119A-BA459

Comments: \_\_\_\_\_  
\_\_\_\_\_  
\_\_\_\_\_

**ORGANICS  
Calibration Data**

TPH Extractables  
DOC1028

Form 6  
Initial Calibration

Lab Name: APPL, Inc.

SDG No: \_\_\_\_\_

Case No: \_\_\_\_\_

Initial Cal. Date: 10/28/2021

Matrix: Water

Instrument: Apollo

Initials: KA

1028003.D    1028004.D    1028005.D    1028006.D    1028007.D    1028008.D    1028009.D

	Compound	1	2	3	4	5	6	7				Avg	%RSD	Type	r <sup>2</sup>	Q
1	HATM Diesel (C10-C24)	2983809	2406563	2517872	2418941	2337993	2387715	2563791				2516669	8.7	HATM		
2	HBTML Motor Oil (C24-C40)	5192328	3260715	2065863	1824592	1695984	1676117	1728658				2492037	53	HBTM	1.000	
3	SA Ortho-Terphenyl(S)	3637234	3178668	3119876	3035678	2926966	2905323	3088794				3127505	7.9	SA		
4	SA Octacosane(S)	2469203	2170507	2286410	2275552	2170413	2171254	2286658				2261428	4.8	SA		
5																
6																
7																
8																
9																
10																
11																
12																
13																
14																
15																
16																
17																
18																
19																
20																
21																
22																
23																
24																
25																
26																
27																
28																
29																
30																
31																
32																
33																
34																
35																

2.118919

Data File : G:\APOLLO\DATA\211028\1028003.D Vial: 3  
 Acq On : 10-28-21 9:19:03 Operator: KA  
 Sample : DMO STD 1 10/28/21 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Oct 28 15:39 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Oct 28 15:39:11 2021  
 Response via : Multiple Level Calibration




Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A

Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.53	1818617	0.291 ppb
Surrogate Spike 30.000		Recovery =	0.97%
4) SA Octacosane(S)	9.82	1234601	0.273 ppb
Surrogate Spike 30.000		Recovery =	0.91%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	29838086	5.928 ppb
2) HBTM Motor Oil (C24-C40)	14.96	51923283	5.234 ppb
Target Compounds			

Quantitation Report

Data File: G:\APOLLO\DATA\211028\1028003.D

Sample : DMO STD 1 10/28/21



Data File : G:\APOLLO\DATA\211028\1028004.D Vial: 4  
 Acq On : 10-28-21 9:47:06 Operator: KA  
 Sample : DMO STD 2 10/28/21 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Oct 28 15:39 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Oct 28 15:39:11 2021  
 Response via : Multiple Level Calibration



Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A

Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.53	3178668	0.508 ppb
Surrogate Spike 30.000		Recovery =	1.69%
4) SA Octacosane(S)	9.82	2170507	0.480 ppb
Surrogate Spike 30.000		Recovery =	1.60%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	48131263	9.562 ppb
2) HBTM Motor Oil (C24-C40)	14.96	65214303	9.152 ppb
Target Compounds			

Quantitation Report

Data File: G:\APOLLO\DATA\211028\1028004.D

Sample : DMO STD 2 10/28/21



Data File : G:\APOLLO\DATA\211028\1028005.D Vial: 5  
 Acq On : 10-28-21 10:15:13 Operator: KA  
 Sample : DMO STD 3 10/28/21 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Oct 28 15:39 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Oct 28 15:39:11 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A



Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.53	15599382	2.494 ppb
Surrogate Spike 30.000		Recovery =	8.31%
4) SA Octacosane(S)	9.82	11432050	2.528 ppb
Surrogate Spike 30.000		Recovery =	8.43%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	251787231	50.024 ppb
2) HBTM Motor Oil (C24-C40)	14.96	206586322	50.832 ppb

Target Compounds



Quantitation Report

Data File: G:\APOLLO\DATA\211028\1028005.D  
Sample : DMO STD 3 10/28/21



Data File : G:\APOLLO\DATA\211028\1028006.D Vial: 6  
 Acq On : 10-28-21 10:43:31 Operator: KA  
 Sample : DMO STD 4 10/28/21 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Oct 28 15:39 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Oct 28 15:39:11 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A



Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.53	75891940	12.133 ppb
Surrogate Spike 30.000		Recovery =	40.44%
4) SA Octacosane(S)	9.82	56888797	12.578 ppb
Surrogate Spike 30.000		Recovery =	41.93%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	1209470396	240.292 ppb
2) HBTM Motor Oil (C24-C40)	14.96	912296132	258.892 ppb

Target Compounds

Quantitation Report

Data File: G:\APOLLO\DATA\211028\1028006.D

Sample : DMO STD 4 10/28/21



Quantitation Report (Not Reviewed)

Data File : G:\APOLLO\DATA\211028\1028007.D Vial: 7  
 Acq On : 10-28-21 11:11:42 Operator: KA  
 Sample : DMO STD 5 10/28/21 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Oct 28 15:39 2021 Quant Results File: DOC1028.RES



Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Oct 28 15:39:11 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A

Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.54	292696553	46.794 ppb
Surrogate Spike 30.000		Recovery =	155.98%
4) SA Octacosane(S)	9.83	217041298	47.988 ppb
Surrogate Spike 30.000		Recovery =	159.96%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	4675985227	929.003 ppb
2) HBTM Motor Oil (C24-C40)	14.96	3391967397	989.959 ppb
Target Compounds			

Quantitation Report

Data File: G:\APOLLO\DATA\211028\1028007.D  
Sample : DMO STD 5 10/28/21



Data File : G:\APOLLO\DATA\211028\1028008.D Vial: 8  
 Acq On : 10-28-21 11:39:55 Operator: KA  
 Sample : DMO STD 6 10/28/21 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Oct 28 15:39 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Oct 28 15:39:11 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A

Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.54	435798382	69.672 ppb
Surrogate Spike 30.000		Recovery =	232.24%
4) SA Octacosane(S)	9.84	325688048	72.009 ppb
Surrogate Spike 30.000		Recovery =	240.03%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	7163144090	1423.140 ppb
2) HBTM Motor Oil (C24-C40)	14.96	5028351305	1472.405 ppb



Target Compounds

Quantitation Report

Data File: G:\APOLLO\DATA\211028\1028008.D

Sample : DMO STD 6 10/28/21

1028008.D\FID1B



Data File : G:\APOLLO\DATA\211028\1028009.D Vial: 9  
 Acq On : 10-28-21 12:08:10 Operator: KA  
 Sample : DMO STD 7 10/28/21 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Oct 28 15:39 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Oct 28 15:39:11 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A

Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.54	617758709	98.762 ppb
Surrogate Spike 30.000		Recovery =	329.21%
4) SA Octacosane(S)	9.85	457331573	101.116 ppb
Surrogate Spike 30.000		Recovery =	337.05%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	10255165539	2037.448 ppb
2) HBTM Motor Oil (C24-C40)	14.96	6914631831	2028.526 ppb



Target Compounds



Quantitation Report

Data File: G:\APOLLO\DATA\211028\1028009.D

Sample : DMO STD 7 10/28/21



TPH Extractables  
DOC1028

Form 7

Second Source Calibration

Lab Name: APPL, Inc.

SDG No: \_\_\_\_\_

Case No: \_\_\_\_\_

Date Analyzed: 10/28/2021

Matrix: Water

Instrument: Apollo

Initial Cal. Date: 10/28/2021

Data File: 1028010.D

		Compound	MEAN	CCRF	%D	%Drift
1	HATM	Diesel (C10-C24)	2516670	2266400	9.9	HATM
2	HBTM	Motor Oil (C24-C40)	2492040	1663520	33	HBTML 5.9
3						
4						
5						
6						
7						
8						
9						
10						
11						
12						
13						
14						
15						
16						
17						
18						
19						
20						
21						
22						
23						
24						
25						
26						
27						
28						
29						
30						
31						
32						
33						
34						
35						
36						
37						
38						
39						
40		Average			21.5	

Data File : G:\APOLLO\DATA\211028\1028010.D Vial: 10  
 Acq On : 10-28-21 12:36:26 Operator: KA  
 Sample : DMO Second Source 10/28/21 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Oct 28 15:39 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Oct 28 15:39:11 2021  
 Response via : Multiple Level Calibration



Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A


Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.53	4250105	0.679 ppb
Surrogate Spike 30.000		Recovery =	2.26%
4) SA Octacosane(S)	9.83	-3553	N.D. ppb
Surrogate Spike 30.000		Recovery =	0.00%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	1133202337	225.139 ppb
2) HBTM Motor Oil (C24-C40)	14.96	831758038	235.148 ppb

Target Compounds

Quantitation Report

Data File: G:\APOLLO\DATA\211028\1028010.D  
Sample : DMO Second Source 10/28/21





Method Name: G:\APOLLO\DATA\211028\DOC1028.M  
 Calibration Table Last Updated: Thu Oct 28 15:37:06 2021

TPH Extractables  
DOC1028

Form 7

Continuing Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Date Analyzed: 11/18/2021  
Instrument: Apollo  
Initial Cal. Date: 10/28/2021  
Data File: 1117080.D

		Compound	MEAN	CCRF	%D		%Drift
1	HATM	Diesel (C10-C24)	2516670	2796810	11	HATM	
2	HBTM	Motor Oil (C24-C40)	2492040	1930360	23	HBTML	9.8
3	SA	Ortho-Terphenyl(S)	3127510	2947660	5.8	SA	
4	SA	Octacosane(S)	2261430	2437230	7.8	SA	
5							
6							
7							
8							
9							
10							
11							
12							
13							
14							
15							
16							
17							
18							
19							
20							
21							
22							
23							
24							
25							
26							
27							
28							
29							
30							
31							
32							
33							
34							
35							
36							
37							
38							
39							
40							

Average

11.9

Data File : G:\APOLLO\DATA\211117\1117080.D Vial: 80  
 Acq On : 11-18-21 22:49:17 Operator: KA  
 Sample : DMO LVL 4 CCV 10/27/21 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Nov 19 10:08 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Nov 18 13:26:01 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A



Compound	R.T.	Response	Conc Units
-----			
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.42	73691447	11.781 ppb
Surrogate Spike 30.000		Recovery =	39.27%
4) SA Octacosane(S)	9.66	60930654	13.472 ppb
Surrogate Spike 30.000		Recovery =	44.91%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	1398406157	277.829 ppb
2) HBTM Motor Oil (C24-C40)	14.96	965178863	274.483 ppb

Target Compounds

Quantitation Report

Data File: G:\APOLLO\DATA\211117\1117080.D

Sample : DMO LVL 4 CCV 10/27/21





TPH Extractables  
DOC1028

Form 7  
Continuing Calibration

Lab Name: APPL, Inc.

SDG No: \_\_\_\_\_

Case No: \_\_\_\_\_

Date Analyzed: 11/19/2021

Matrix: Water

Instrument: Apollo

Initial Cal. Date: 10/28/2021

Data File: 1117092.D

	Compound	MEAN	CCRF	%D	%Drift	
1	HATM Diesel (C10-C24)	2516670	2750900	9.3	HATM	
2	HBTM Motor Oil (C24-C40)	2492040	1875410	25	HBTML	6.6
3	SA Ortho-Terphenyl(S)	3127510	2920050	6.6	SA	
4	SA Octacosane(S)	2261430	2407500	6.5	SA	
5						
6						
7						
8						
9						
10						
11						
12						
13						
14						
15						
16						
17						
18						
19						
20						
21						
22						
23						
24						
25						
26						
27						
28						
29						
30						
31						
32						
33						
34						
35						
36						
37						
38						
39						
40	Average			11.9		

Quantitation Report (Not Reviewed)

Data File : G:\APOLLO\DATA\211117\1117092.D Vial: 92  
 Acq On : 11-19-21 4:26:09 Operator: KA  
 Sample : DMO LVL 4 CCV 10/27/21 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Nov 19 10:09 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Nov 18 13:26:01 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A

Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.42	73001201	11.671 ppb
Surrogate Spike 30.000		Recovery =	38.90%
4) SA Octacosane(S)	9.65	60187569	13.307 ppb
Surrogate Spike 30.000		Recovery =	44.36%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	1375448848	273.268 ppb
2) HBTM Motor Oil (C24-C40)	14.96	937704588	266.383 ppb



Target Compounds

Quantitation Report

Data File: G:\APOLLO\DATA\211117\1117092.D

Sample : DMO LVL 4 CCV 10/27/21

1117092.D\FID1B



**ORGANICS**  
**Raw Data**

Data File : G:\APOLLO\DATA\211117\1117089.D Vial: 89  
 Acq On : 11-19-21 3:01:57 Operator: KA  
 Sample : BA46115W09 5/1040 Inst : Apollo  
 Misc : water Multiplr: 4.81  
 IntFile : events.e  
 Quant Time: Nov 19 18:14 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Nov 18 13:26:01 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A



Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.42	143892735	110.598 ppb
Surrogate Spike 144.231		Recovery =	76.68%
4) SA Octacosane(S)	9.66	129921581	138.104 ppb
Surrogate Spike 144.231		Recovery =	95.75%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	47334872	45.213 ppb
2) HBTM Motor Oil (C24-C40)	14.96	245205453	299.125 ppb

Target Compounds

Quantitation Report

Data File: G:\APOLLO\DATA\211117\1117089.D

Sample : BA46115W09 5/1040



Data File : G:\APOLLO\DATA\211117\1117090.D Vial: 90  
 Acq On : 11-19-21 3:30:02 Operator: KA  
 Sample : BA46116W07 5/1020 Inst : Apollo  
 Misc : water Multiplr: 4.90  
 IntFile : events.e  
 Quant Time: Nov 19 18:15 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Nov 18 13:26:01 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A



Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.42	142100513	111.362 ppb
Surrogate Spike 147.059		Recovery =	75.73%
4) SA Octacosane(S)	9.65	128526465	139.299 ppb
Surrogate Spike 147.059		Recovery =	94.72%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	61067121	59.473 ppb
2) HBTM Motor Oil (C24-C40)	14.96	222760390	272.552 ppb

Target Compounds

Quantitation Report

Data File: G:\APOLLO\DATA\211117\1117090.D

Sample : BA46116W07 5/1020





Data File : G:\APOLLO\DATA\211117\1117081.D Vial: 81  
 Acq On : 11-18-21 23:17:21 Operator: KA  
 Sample : 211116A BLK 5/1000 Inst : Apollo  
 Misc : water Multiplr: 5.00  
 IntFile : events.e  
 Quant Time: Nov 19 18:11 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Nov 18 13:26:01 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A



Compound	R.T.	Response	Conc Units
<b>System Monitoring Compounds</b>			
3) SA Ortho-Terphenyl (S)	7.42	137256500	109.717 ppb
Surrogate Spike 150.000		Recovery =	73.14%
4) SA Octacosane (S)	9.66	123210935	136.209 ppb
Surrogate Spike 150.000		Recovery =	90.81%
<b>Target Compounds</b>			
1) HATM Diesel (C10-C24)	6.49	36368663	36.128 ppb
2) HBTM Motor Oil (C24-C40)	14.96	261607938	335.269 ppb

Target Compounds

Quantitation Report

Data File: G:\APOLLO\DATA\211117\1117081.D

Sample : 211116A BLK 5/1000



Quantitation Report (QT Reviewed)

Data File : G:\APOLLO\DATA\211117\1117082.D Vial: 82  
 Acq On : 11-18-21 23:45:25 Operator: KA  
 Sample : 211116A LCS-1 5/1000 Inst : Apollo  
 Misc : water Multiplr: 5.00  
 IntFile : events.e  
 Quant Time: Nov 19 18:11 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Nov 18 13:26:01 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A

Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.42	161516467	129.110 ppb
Surrogate Spike 150.000		Recovery =	86.07%
4) SA Octacosane(S)	9.66	128589047	142.155 ppb
Surrogate Spike 150.000		Recovery =	94.77%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	1849571519	1837.321 ppb
2) HBTM Motor Oil (C24-C40)	14.96	1314792569	1887.790 ppb
Target Compounds			



Diesel:

$$\frac{(1849571519)(5)}{(2516669)(2)} = \frac{9247857595}{5033338} = \boxed{1837.321}$$

Quantitation Report

Data File: G:\APOLLO\DATA\211117\1117082.D

Sample : 211116A LCS-1 5/1000



Data File : G:\APOLLO\DATA\211117\1117083.D Vial: 83  
 Acq On : 11-19-21 0:13:29 Operator: KA  
 Sample : 211116A LCSD-1 5/1000 Inst : Apollo  
 Misc : water Multiplr: 5.00  
 IntFile : events.e  
 Quant Time: Nov 19 18:12 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Nov 18 13:26:01 2021  
 Response via : Multiple Level Calibration



Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A

Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.42	159977422	127.879 ppb
Surrogate Spike 150.000		Recovery =	85.25%
4) SA Octacosane(S)	9.66	128713604	142.292 ppb
Surrogate Spike 150.000		Recovery =	94.86%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	1781600131	1769.800 ppb
2) HBTM Motor Oil (C24-C40)	14.96	1319942855	1895.382 ppb

Target Compounds

Quantitation Report

Data File: G:\APOLLO\DATA\211117\1117083.D  
Sample : 211116A LCSD-1 5/1000



## Diesel / Motor Oil Calibration Curve

Prepared: 10/28/2021

Expires: 5/31/2026

Prepared By (Initials): KA

Methylene

e

Chloride

Lot No. 61117

Initial Standard Information							Final Standard			
Name of Initial Standard (QAU Label)	Supplier	Conc. (ug/mL)	APPL Mix Name	Reference to APPL Prep Date and Lot #'s	Exp. Date	Exp. Date (Manufacturer)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/mL)
Diesel / Motor Oil - 2	APPL	10	Diesel / Motor Oil - 1	Prep'd: 10/6/21 A0164485-52822, A0168842-52820, A0166510-52817 CL16893-52835	See man. Exp date	10/31/2027 12/31/2027 5/31/2026	100uL	200uL	MC	5
Diesel / Motor Oil - 3		50	Diesel / Motor Oil - 2				200uL	1mL	MC	10
Diesel / Motor Oil Calibration STD	Restek	2,000	Diesel / Motor Oil - 3				25uL	1mL	MC	50
			Diesel / Motor Oil - 4				125uL	1mL	MC	250
			Diesel / Motor Oil - 5				500uL	1mL	MC	1000
			Diesel / Motor Oil - 6				750uL	1mL	MC	1500
			Diesel / Motor Oil - 7				100uL	100uL	N/A	2,000

### Diesel / Motor Oil Second Source

Prepared: 10/28/2021

Expires: 10/28/2024

Prepared By (Initials): KA

Methylene

e

Chloride

Lot No. 61117

Initial Standard Information							Final Standard			
Name of Initial Standard (QAU Label)	Supplier	Supplier Part No.	Conc. (ug/mL)	Lot Number - QA Number	Exp. Date (1 yr.)	Exp. Date (Manufacturer)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/mL)
Diesel Fuel #2 Second Source	Phenova	AL0-101287	50,000	CL16477-52980	See man. Exp date	2/28/2027	50uL	10mL	MC	250
Motor Oil Second Source	Absolute	51094	50,000	102819-52981		10/28/2024	50uL			



**Diesel / Motor Oil CCV**

Prepared: 10/27/2021

Expires: 5/31/2026

Prepared By (Initials): KA

Methylen

e

Chloride

Lot No. 61117

Initial Standard Information							Final Standard			
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference to APPL Prep Date and Lot #'s	Exp. Date	Exp. Date (Manufacturer)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/mL)
Diesel / Motor Oil STD	Restek	Diesel / Motor Oil CCV	2,000	Perp'd: 10/06/21 A0164485-52822, A0168842-52820, A0166510-52817, CL16893-52835	See man. Exp date	10/31/2027 12/31/2027 5/31/2026	1250uL	10mL	MC	250

**Diesel Motor Oil Mix**

Prepared: 10/30/2021

Prepared By (Initials): KA

Expires: 10/31/2027

Initial Standard Information							Final Standard			
Name of Initial Standard (QAU Label)	Supplier	Supplier Part No.	Conc. (ug/mL)	Lot Number - QA Number	Exp. Date (1 yr.)	Exp. Date (Manufacturer)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/mL)
Diesel Fuel #2	Restek	31258	50,000	A0164485-52825 and A0164586-53175, 53174, and 53176	See man. Date	10/31/2027	4.00 mL	8.0 mL	NA	25,000
Motor Oil Composite	Restek	31464	50,000	A0166510-52817, and A0168842-53169, 53170, and 53171	See man. Date	12/31/2027 3/31/28	4.00 mL			25,000

**THC Surrogate****Prepared: 11/10/2021****KA****Expires: 5/31/2026**

Initial Standard Information							Final Standard			
Name of Initial Standard (QAU Label)	Supplier	Supplier Part No.	Conc. (ug/mL)	Lot Number - QA Number	Exp. Date (1 yr.)	Exp. Date (Manufacturer)	Allquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/mL)
O-terphenyl / Octacosane Mix	Phenova	ALO-130161	600	CL16893-52839	See man. Date	5/31/2026	N/A	N/A	N/A	600

# Organic Extraction Worksheet

<b>Method</b>	Continuous Liq/Liq TPH- 3520C w/SGC	<b>Extraction Set</b>	211116A	<b>Extraction Method</b>	LIQ005SGC	<b>Units</b>	mL
Spiked ID 1	Diesel Motor Oil Mix 10-30-21 10-31-27	Surrogate ID 1	THC Surrogate 11-10-21 11-10-22				
Spiked ID 2	Decanoic 1000ug/mL Acid Solution 11-5-21 11-5-22	Surrogate ID 2					
Spiked ID 3		Surrogate ID 3					
Spiked ID 4		Surrogate ID 4					
Spiked ID 5		Surrogate ID 5					
Spiked ID 6		Sufficient Vol for Matrix QC:		NO			
Spiked ID 7		Ext. Start Time:		11/16/21 13:42			
Spiked ID 8		Ext. End Time:		11/17/21 7:48			
<b>GC Requires Extract By:</b>							
pH1	2	11/16/21 12:10	Water Bath Temp 1 °C	35/34.1 °C			
pH2			Water Bath Temp 2 °C	35/36.1			
pH3			Water Bath Temp 3 °C	35/35.5 °C			

Spiked By: SR

Date 11/16/2021

Witnessed By: CG

Date 11/16/2021

Sample	Sample Container	Spike Amount	Spike ID	Surrogate Amount	Surrogate ID	Extract Amount	Final Volume	pH	Extract Date/Time	Comments
1	211116A Blk	0.050	2	0.250	1	1000	5	2	11/16/21 12:12	*
					equip	E-HP3 E-WB1				
2	211116A LCS-1	0.080,0.050	1,2	0.250	1	1000	5	2	11/16/21 12:12	*
					equip	E-HP4 E-WB2				
3	211116A LCSD-1	0.080,0.050	1,2	0.250	1	1000	5	2	11/16/21 12:12	*
					equip	E-HP6 E-WB3				
4	BA46001 BA46001W09	0.050	2	0.250	1	1020	5	2	11/16/21 12:12	98213 *
					equip	E-HP7 E-WB1				
5	BA46103 BA46103W09	0.050	2	0.250	1	1020	5	2	11/16/21 12:12	98214 *
					equip	E-HP8 E-WB2				
6	BA46105 BA46105W09	0.050	2	0.250	1	1040	5	2	11/16/21 12:12	98214 *
					equip	E-HP9 E-WB3				
7	BA46107 BA46107W09	0.050	2	0.250	1	1050	5	2	11/16/21 12:12	98214 *
					equip	E-HP10 E-WB1				
8	BA46109 BA46109W09	0.050	2	0.250	1	1010	5	2	11/16/21 12:12	98214 *
					equip	E-HP11 E-WB2				
9	BA46115 BA46115W09	0.050	2	0.250	1	1040	5	2	11/16/21 12:12	98212 *
					equip	E-HP12 E-WB3				
10	BA46116 BA46116W07	0.050	2	0.250	1	1020	5	2	11/16/21 12:12	98212 *
					equip	E-HP13 E-WB1				
11	BA46117 BA46117W03	0.050	2	0.250	1	1020	5	2	11/16/21 12:12	98212 *
					equip	E-HP14 E-WB2				

Solvent and Lot#	
1+1 HCL (5mLs)	60358
PH Strips	HC155968
Dichloromethane (DCM)	61117
Filter Paper	400202
Sodium Sulfate	2021071206
SILICA GEL (*)	050627T

Extraction COC Transfer	
Extraction lab employee Initials	KY
GC analyst's initials	KA
Date	11/18/21
Time	10:48
Refrigerator	HOBART

Technician's Initials	
Scanned By	SR
Sample Preparation	SR
Extraction	SR
Concentration	SR,DS
Modified	11/18/2021 7:17:39 AM

Reviewed By: KY

Date 11/18/2021

## Injection Log

Directory: G:\APOLLO\DATA\211028\

Line	Vial	FileName	Multiplier	SampleName	Misc Info	Injected
1	3	1028003.D	1	DMO STD 1 10/28/21	water	10-28-21 9:19:03
2	4	1028004.D	1	DMO STD 2 10/28/21	water	10-28-21 9:47:06
3	5	1028005.D	1	DMO STD 3 10/28/21	water	10-28-21 10:15:13
4	6	1028006.D	1	DMO STD 4 10/28/21	water	10-28-21 10:43:31
5	7	1028007.D	1	DMO STD 5 10/28/21	water	10-28-21 11:11:42
6	8	1028008.D	1	DMO STD 6 10/28/21	water	10-28-21 11:39:55
7	9	1028009.D	1	DMO STD 7 10/28/21	water	10-28-21 12:08:10
8	10	1028010.D	1	DMO Second Source 10/28/21	water	10-28-21 12:36:26
9	80	1117080.D	1	DMO LVL 4 CCV 10/27/21	water	11-18-21 22:49:17
10	81	1117081.D	5	211116A BLK 5/1000	water	11-18-21 23:17:21
11	82	1117082.D	5	211116A LCS-1 5/1000	water	11-18-21 23:45:25
12	83	1117083.D	5	211116A LCSD-1 5/1000	water	11-19-21 0:13:29
13	89	1117089.D	4.80769	BA46115W09 5/1040	water	11-19-21 3:01:57
14	90	1117090.D	4.90196	BA46116W07 5/1020	water	11-19-21 3:30:02
15	91	1117091.D	4.90196	BA46117W03 5/1020	water	11-19-21 3:58:03
16	92	1117092.D	1	DMO LVL 4 CCV 10/27/21	water	11-19-21 4:26:09

**ORGANICS**  
**Calibration Data**

TPH Extractables  
DOC1028

Form 6  
Initial Calibration

Lab Name: APPL, Inc.

SDG No: \_\_\_\_\_

Case No: \_\_\_\_\_

Initial Cal. Date: 10/28/2021

Matrix: Water

Instrument: Apollo

Initials: KA

1028003.D    1028004.D    1028005.D    1028006.D    1028007.D    1028008.D    1028009.D

	Compound	1	2	3	4	5	6	7				Avg	%RSD	Type	r <sup>2</sup>	Q
1	HATM Diesel (C10-C24)	2983809	2406563	2517872	2418941	2337993	2367715	2563791				2516669	8.7	HATM		
2	HBTML Motor Oil (C24-C40)	5192328	3260715	2065863	1824592	1695984	1676117	1728658				2492037	53	HBTM	1.000	
3	SA Ortho-Terphenyl(S)	3637234	3178668	3119876	3035678	2926966	2905323	3088794				3127505	7.9	SA		
4	SA Octacosane(S)	2469203	2170507	2286410	2275552	2170413	2171254	2286658				2261428	4.8	SA		
5																
6																
7																
8																
9																
10																
11																
12																
13																
14																
15																
16																
17																
18																
19																
20																
21																
22																
23																
24																
25																
26																
27																
28																
29																
30																
31																
32																
33																
34																
35																

2.118919

Data File : G:\APOLLO\DATA\211028\1028003.D Vial: 3  
 Acq On : 10-28-21 9:19:03 Operator: KA  
 Sample : DMO STD 1 10/28/21 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Oct 28 15:39 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Oct 28 15:39:11 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A

Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.53	1818617	0.291 ppb
Surrogate Spike 30.000		Recovery =	0.97%
4) SA Octacosane(S)	9.82	1234601	0.273 ppb
Surrogate Spike 30.000		Recovery =	0.91%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	29838086	5.928 ppb
2) HBTM Motor Oil (C24-C40)	14.96	51923283	5.234 ppb



Target Compounds



Quantitation Report

Data File: G:\APOLLO\DATA\211028\1028003.D

Sample : DMO STD 1 10/28/21



Data File : G:\APOLLO\DATA\211028\1028004.D Vial: 4  
 Acq On : 10-28-21 9:47:06 Operator: KA  
 Sample : DMO STD 2 10/28/21 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Oct 28 15:39 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Oct 28 15:39:11 2021  
 Response via : Multiple Level Calibration



Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A

Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.53	3178668	0.508 ppb
Surrogate Spike 30.000		Recovery =	1.69%
4) SA Octacosane(S)	9.82	2170507	0.480 ppb
Surrogate Spike 30.000		Recovery =	1.60%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	48131263	9.562 ppb
2) HBTM Motor Oil (C24-C40)	14.96	65214303	9.152 ppb
Target Compounds			

Quantitation Report

Data File: G:\APOLLO\DATA\211028\1028004.D

Sample : DMO STD 2 10/28/21



Quantitation Report (Not Reviewed)

Data File : G:\APOLLO\DATA\211028\1028005.D Vial: 5  
 Acq On : 10-28-21 10:15:13 Operator: KA  
 Sample : DMO STD 3 10/28/21 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Oct 28 15:39 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Oct 28 15:39:11 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A



Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.53	15599382	2.494 ppb
Surrogate Spike 30.000		Recovery =	8.31%
4) SA Octacosane(S)	9.82	11432050	2.528 ppb
Surrogate Spike 30.000		Recovery =	8.43%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	251787231	50.024 ppb
2) HBTM Motor Oil (C24-C40)	14.96	206586322	50.832 ppb

Target Compounds

Quantitation Report

Data File: G:\APOLLO\DATA\211028\1028005.D

Sample : DMO STD 3 10/28/21



Data File : G:\APOLLO\DATA\211028\1028006.D Vial: 6  
 Acq On : 10-28-21 10:43:31 Operator: KA  
 Sample : DMO STD 4 10/28/21 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Oct 28 15:39 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Oct 28 15:39:11 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A



Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.53	75891940	12.133 ppb
Surrogate Spike 30.000		Recovery =	40.44%
4) SA Octacosane(S)	9.82	56888797	12.578 ppb
Surrogate Spike 30.000		Recovery =	41.93%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	1209470396	240.292 ppb
2) HBTM Motor Oil (C24-C40)	14.96	912296132	258.892 ppb

Target Compounds

Quantitation Report

Data File: G:\APOLLO\DATA\211028\1028006.D

Sample : DMO STD 4 10/28/21



Quantitation Report (Not Reviewed)

Data File : G:\APOLLO\DATA\211028\1028007.D Vial: 7  
 Acq On : 10-28-21 11:11:42 Operator: KA  
 Sample : DMO STD 5 10/28/21 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Oct 28 15:39 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Oct 28 15:39:11 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A

Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.54	292696553	46.794 ppb
Surrogate Spike 30.000		Recovery =	155.98%
4) SA Octacosane(S)	9.83	217041298	47.988 ppb
Surrogate Spike 30.000		Recovery =	159.96%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	4675985227	929.003 ppb
2) HBTM Motor Oil (C24-C40)	14.96	3391967397	989.959 ppb



Target Compounds



Quantitation Report

Data File: G:\APOLLO\DATA\211028\1028007.D

Sample : DMO STD 5 10/28/21



Quantitation Report (Not Reviewed)

Data File : G:\APOLLO\DATA\211028\1028008.D Vial: 8  
 Acq On : 10-28-21 11:39:55 Operator: KA  
 Sample : DMO STD 6 10/28/21 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Oct 28 15:39 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Oct 28 15:39:11 2021  
 Response via : Multiple Level Calibration



Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A

Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.54	435798382	69.672 ppb
Surrogate Spike 30.000		Recovery =	232.24%
4) SA Octacosane(S)	9.84	325688048	72.009 ppb
Surrogate Spike 30.000		Recovery =	240.03%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	7163144090	1423.140 ppb
2) HBTM Motor Oil (C24-C40)	14.96	5028351305	1472.405 ppb

Target Compounds

Quantitation Report

Data File: G:\APOLLO\DATA\211028\1028008.D  
Sample : DMO STD 6 10/28/21



Data File : G:\APOLLO\DATA\211028\1028009.D Vial: 9  
 Acq On : 10-28-21 12:08:10 Operator: KA  
 Sample : DMO STD 7 10/28/21 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Oct 28 15:39 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Oct 28 15:39:11 2021  
 Response via : Multiple Level Calibration



Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A

Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.54	617758709	98.762 ppb
Surrogate Spike 30.000		Recovery =	329.21%
4) SA Octacosane(S)	9.85	457331573	101.116 ppb
Surrogate Spike 30.000		Recovery =	337.05%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	10255165539	2037.448 ppb
2) HBTM Motor Oil (C24-C40)	14.96	6914631831	2028.526 ppb
Target Compounds			

Quantitation Report

Data File: G:\APOLLO\DATA\211028\1028009.D

Sample : DMO STD 7 10/28/21



TPH Extractables  
DOC1028

Form 7

Second Source Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Date Analyzed: 10/28/2021  
Instrument: Apollo  
Initial Cal. Date: 10/28/2021  
Data File: 1028010.D

	Compound	MEAN	CCRF	%D	%Drift	
1	HATM Diesel (C10-C24)	2516670	2266400	9.9	HATM	
2	HBTM Motor Oil (C24-C40)	2492040	1663520	33	HBTML	5.9
3						
4						
5						
6						
7						
8						
9						
10						
11						
12						
13						
14						
15						
16						
17						
18						
19						
20						
21						
22						
23						
24						
25						
26						
27						
28						
29						
30						
31						
32						
33						
34						
35						
36						
37						
38						
39						
40	Average			21.5		

Quantitation Report (Not Reviewed)

Data File : G:\APOLLO\DATA\211028\1028010.D Vial: 10  
 Acq On : 10-28-21 12:36:26 Operator: KA  
 Sample : DMO Second Source 10/28/21 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Oct 28 15:39 2021 Quant Results File: DOC1028.RES



Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Oct 28 15:39:11 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A


Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.53	4250105	0.679 ppb
Surrogate Spike 30.000		Recovery =	2.26%
4) SA Octacosane(S)	9.83	-3553	N.D. ppb
Surrogate Spike 30.000		Recovery =	0.00%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	1133202337	225.139 ppb
2) HBTM Motor Oil (C24-C40)	14.96	831758038	235.148 ppb
Target Compounds			

Quantitation Report

Data File: G:\APOLLO\DATA\211028\1028010.D  
Sample : DMO Second Source 10/28/21







Method Name: G:\APOLLO\DATA\211028\DOC1028.M  
 Calibration Table Last Updated: Thu Oct 28 15:37:06 2021

TPH Extractables  
DEC0911

Form 6  
Initial Calibration

Lab Name: APPL, Inc.

SDG No: \_\_\_\_\_

Case No: \_\_\_\_\_

Initial Cal. Date: 9/11/2021

Matrix: Water

Instrument: Apollo

Initials: KA

911002.D    911003.D    911004.D    911005.D    911006.D    911007.D

	Compound	1	2	3	4	5	6						Avg	%RSD	Type	r <sup>2</sup>	Q
1	SC Decanoic Acid(S)	883995	1084261	1313446	1384667	1522107	1509937						1283069	20	SC		*
2																	
3																	
4																	
5																	
6																	
7																	
8																	
9																	
10																	
11																	
12																	
13																	
14																	
15																	
16																	
17																	
18																	
19																	
20																	
21																	
22																	
23																	
24																	
25																	
26																	
27																	
28																	
29																	
30																	
31																	
32																	
33																	
34																	
35																	

0.562142

Data File : G:\APOLLO\DATA\210911\911002.D Vial: 2  
 Acq On : 9-11-21 10:22:53 Operator: KA  
 Sample : Decanoic Acid STD 1 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Sep 13 9:30 2021 Quant Results File: DEC0911.RES

Method : G:\APOLLO\DATA\210808\DEC0911.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Mon Sep 13 09:30:16 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A


Compound	R.T.	Response	Conc Units
-----			
System Monitoring Compounds			
1) SC Decanoic Acid(S)	5.77	5303968	2.067 ppb
Surrogate Spike 24.000	Recovery	=	8.61%
Target Compounds			
Target Compounds			

Quantitation Report

Data File: G:\APOLLO\DATA\210911\911002.D

Sample : Decanoic Acid STD 1

911002.D\FID1B



Quantitation Report (Not Reviewed)

Data File : G:\APOLLO\DATA\210911\911003.D Vial: 3  
 Acq On : 9-11-21 10:51:11 Operator: KA  
 Sample : Decanoic Acid STD 2 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Sep 23 17:12 2021 Quant Results File: DEC0911.RES

Method : G:\APOLLO\DATA\210808\DEC0911.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Mon Sep 13 09:30:16 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A

Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
1) SC Decanoic Acid(S)	5.77	13011132	5.070 ppb
Surrogate Spike 24.000		Recovery =	21.13%


Target Compounds

Target Compounds

Quantitation Report

Data File: G:\APOLLO\DATA\210911\911003.D

Sample : Decanoic Acid STD 2



Quantitation Report (Not Reviewed)

Data File : G:\APOLLO\DATA\210911\911004.D Vial: 4  
 Acq On : 9-11-21 11:19:39 Operator: KA  
 Sample : Decanoic Acid STD 3 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Sep 23 17:12 2021 Quant Results File: DEC0911.RES

Method : G:\APOLLO\DATA\210808\DEC0911.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Mon Sep 13 09:30:16 2021  
 Response via : Multiple Level Calibration


Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A

Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
1) SC Decanoic Acid(S)	5.79	63045408	24.568 ppb
Surrogate Spike 24.000		Recovery =	102.37%
Target Compounds			
Target Compounds			

Quantitation Report

Data File: G:\APOLLO\DATA\210911\911004.D

Sample : Decanoic Acid STD 3





Data File : G:\APOLLO\DATA\210911\911005.D Vial: 5  
 Acq On : 9-11-21 11:48:04 Operator: KA  
 Sample : Decanoic Acid STD 4 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Sep 23 17:12 2021 Quant Results File: DEC0911.RES


Method : G:\APOLLO\DATA\210808\DEC0911.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Mon Sep 13 09:30:16 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A

Compound	R.T.	Response	Conc Units
-----			
System Monitoring Compounds			
1) SC Decanoic Acid(S)	5.80	99696015	38.851 ppb
Surrogate Spike 24.000		Recovery =	161.88%
Target Compounds			
Target Compounds			

Data File: G:\APOLLO\DATA\210911\911005.D

Sample : Decanoic Acid STD 4



Data File : G:\APOLLO\DATA\210911\911006.D Vial: 6  
 Acq On : 9-11-21 12:16:37 Operator: KA  
 Sample : Decanoic Acid STD 5 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Sep 23 17:12 2021 Quant Results File: DEC0911.RES

Method : G:\APOLLO\DATA\210808\DEC0911.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Mon Sep 13 09:30:16 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds			
1) SC Decanoic Acid(S)	5.81	146122260	56.942 ppb
Surrogate Spike 24.000		Recovery =	237.26%


Target Compounds

Target Compounds

Quantitation Report

Data File: G:\APOLLO\DATA\210911\911006.D

Sample : Decanoic Acid STD 5



Data File : G:\APOLLO\DATA\210911\911007.D Vial: 7  
 Acq On : 9-11-21 12:45:02 Operator: KA  
 Sample : Decanoic Acid STD 6 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Sep 23 17:12 2021 Quant Results File: DEC0911.RES

Method : G:\APOLLO\DATA\210808\DEC0911.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Mon Sep 13 09:30:16 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

1) SC Decanoic Acid(S)	5.81	181192435	70.609 ppb
Surrogate Spike 24.000		Recovery =	294.20%


Target Compounds

Target Compounds

Data File: G:\APOLLO\DATA\210911\911007.D

Sample : Decanoic Acid STD 6

911007.D\FID1B



TPH Extractables  
DOC1028

Form 7  
Continuing Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Date Analyzed: 11/19/2021  
Instrument: Apollo  
Initial Cal. Date: 10/28/2021  
Data File: 1117092.D

		Compound	MEAN	CCRF	%D	%Drift	
1	HATM	Diesel (C10-C24)	2516670	2750900	9.3	HATM	
2	HBTM	Motor Oil (C24-C40)	2492040	1875410	25	HBTML	6.6
3	SA	Ortho-Terphenyl(S)	3127510	2920050	6.6	SA	
4	SA	Octacosane(S)	2261430	2407500	6.5	SA	
5							
6							
7							
8							
9							
10							
11							
12							
13							
14							
15							
16							
17							
18							
19							
20							
21							
22							
23							
24							
25							
26							
27							
28							
29							
30							
31							
32							
33							
34							
35							
36							
37							
38							
39							
40							

Average

11.9

Data File : G:\APOLLO\DATA\211117\1117092.D Vial: 92  
 Acq On : 11-19-21 4:26:09 Operator: KA  
 Sample : DMO LVL 4 CCV 10/27/21 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Nov 19 10:09 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Nov 18 13:26:01 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A



Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.42	73001201	11.671 ppb
Surrogate Spike 30.000		Recovery =	38.90%
4) SA Octacosane(S)	9.65	60187569	13.307 ppb
Surrogate Spike 30.000		Recovery =	44.36%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	1375448848	273.268 ppb
2) HBTM Motor Oil (C24-C40)	14.96	937704588	266.383 ppb
Target Compounds			



Quantitation Report

Data File: G:\APOLLO\DATA\211117\1117092.D

Sample : DMO LVL 4 CCV 10/27/21



TPH Extractables  
DEC0911

Form 7

Continuing Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Date Analyzed: 11/19/2021  
Instrument: Apollo  
Initial Cal. Date: 9/11/2021  
Data File: 1117093.D

		Compound	MEAN	CCRF	%D	%Drift
1	SC	Decanoic Acid(S)	1283070	1441670	12	SC
2						
3						
4						
5						
6						
7						
8						
9						
10						
11						
12						
13						
14						
15						
16						
17						
18						
19						
20						
21						
22						
23						
24						
25						
26						
27						
28						
29						
30						
31						
32						
33						
34						
35						
36						
37						
38						
39						
40						

Average

12.0

Quantitation Report (Not Reviewed)

Data File : G:\APOLLO\DATA\211117\1117093.D Vial: 93  
 Acq On : 11-19-21 4:54:12 Operator: KA  
 Sample : Decanoic Acid CCV 11/05/21 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Nov 19 10:10 2021 Quant Results File: DEC0911.RES

Method : G:\APOLLO\DATA\210911\DEC0911.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Fri Nov 05 10:50:06 2021  
 Response via : Multiple Level Calibration


Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A

Compound	R.T.	Response	Conc Units
-----			
System Monitoring Compounds			
1) SC Decanoic Acid(S)	5.64	103800237	40.450 ppb
Surrogate Spike 24.000		Recovery =	168.54%

Target Compounds

Target Compounds

File : G:\APOLLO\DATA\211117\1117093.D  
Operator : KA  
Acquired : 11-19-21 4:54:12 using AcqMethod TPHSN.M  
Instrument : Apollo  
Sample Name: Decanoic Acid CCV 11/05/21  
Misc Info : water  
Vial Number: 93



TPH Extractables  
DOC1028

Form 7

Continuing Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Date Analyzed: 11/19/2021  
Instrument: Apollo  
Initial Cal. Date: 10/28/2021  
Data File: 1117106.D

		Compound	MEAN	CCRF	%D	%Drift	
1	HATM	Diesel (C10-C24)	2516670	2794060	11	HATM	
2	HBTM	Motor Oil (C24-C40)	2492040	1930260	23	HBTML	9.8
3	SA	Ortho-Terphenyl(S)	3127510	3434980	9.8	SA	
4	SA	Octacosane(S)	2261430	2442520	8.0	SA	
5							
6							
7							
8							
9							
10							
11							
12							
13							
14							
15							
16							
17							
18							
19							
20							
21							
22							
23							
24							
25							
26							
27							
28							
29							
30							
31							
32							
33							
34							
35							
36							
37							
38							
39							
40							

Average

13.0

Data File : G:\APOLLO\DATA\211117\1117106.D Vial: 6  
 Acq On : 11-19-21 10:58:57 Operator: KA  
 Sample : DMO LVL 4 CCV 10/27/21 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Nov 19 18:54 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Nov 18 13:26:01 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A



Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.42	85874528	13.729 ppb
Surrogate Spike 30.000		Recovery =	45.76%
4) SA Octacosane(S)	9.65	61062951	13.501 ppb
Surrogate Spike 30.000		Recovery =	45.00%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	1397032062	277.556 ppb
2) HBTM Motor Oil (C24-C40)	14.96	965131794	274.470 ppb

Target Compounds

Quantitation Report

Data File: G:\APOLLO\DATA\211117\1117106.D

Sample : DMO LVL 4 CCV 10/27/21



TPH Extractables  
DEC0911

Form 7

Continuing Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Date Analyzed: 11/19/2021  
Instrument: Apollo  
Initial Cal. Date: 9/11/2021  
Data File: 1117107.D

		Compound	MEAN	CCRF	%D	%Drift
1	SC	Decanoic Acid(S)	1283070	1273520	0.74	SC
2						
3						
4						
5						
6						
7						
8						
9						
10						
11						
12						
13						
14						
15						
16						
17						
18						
19						
20						
21						
22						
23						
24						
25						
26						
27						
28						
29						
30						
31						
32						
33						
34						
35						
36						
37						
38						
39						
40		Average			0.7	



Data File : G:\APOLLO\DATA\211117\1117107.D Vial: 7  
 Acq On : 11-19-21 11:26:58 Operator: KA  
 Sample : Decanoic Acid CCV 11/05/21 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Nov 19 18:54 2021 Quant Results File: DEC0911.RES

Method : G:\APOLLO\DATA\210911\DEC0911.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Fri Nov 05 10:50:06 2021  
 Response via : Multiple Level Calibration


Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A

Compound	R.T.	Response	Conc Units
-----			
System Monitoring Compounds			
1) SC Decanoic Acid(S)	5.63	91693244	35.732 ppb
Surrogate Spike 24.000		Recovery =	148.88%

Target Compounds

Target Compounds

File : G:\APOLLO\DATA\211117\1117107.D  
Operator : KA  
Acquired : 11-19-21 11:26:58 using AcqMethod TPHSN.M  
Instrument : Apollo  
Sample Name: Decanoic Acid CCV 11/05/21  
Misc Info : water  
Vial Number: 7



**ORGANICS**  
**Raw Data**

Data File : G:\APOLLO\DATA\211117\1117103.D Vial: 3  
 Acq On : 11-19-21 9:34:44 Operator: KA  
 Sample : BA46115W09 5/1040 SG Inst : Apollo  
 Misc : water Multiplr: 4.81  
 IntFile : events.e  
 Quant Time: Nov 19 18:52 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Nov 18 13:26:01 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A



Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.42	129902147	99.845 ppb
Surrogate Spike 144.231		Recovery =	69.23%
4) SA Octacosane(S)	9.65	117748505	125.164 ppb
Surrogate Spike 144.231		Recovery =	86.78%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	32347182	30.897 ppb
2) HBTM Motor Oil (C24-C40)	14.96	119527582	120.986 ppb

Target Compounds

Quantitation Report

Data File: G:\APOLLO\DATA\211117\1117103.D

Sample : BA46115W09 5/1040 SG



Data File : G:\APOLLO\DATA\211117\1117104.D Vial: 4  
 Acq On : 11-19-21 10:02:48 Operator: KA  
 Sample : BA46116W07 5/1020 SG Inst : Apollo  
 Misc : water Multiplr: 4.90  
 IntFile : events.e  
 Quant Time: Nov 19 18:52 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Nov 18 13:26:01 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A



Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.42	164036076	128.553 ppb
Surrogate Spike 147.059		Recovery =	87.42%
4) SA Octacosane(S)	9.65	147154775	159.489 ppb
Surrogate Spike 147.059		Recovery =	108.45%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	29352842	28.587 ppb
2) HBTM Motor Oil (C24-C40)	14.96	125987100	132.694 ppb

Target Compounds

Quantitation Report

Data File: G:\APOLLO\DATA\211117\1117104.D

Sample : BA46116W07 5/1020 SG



Data File : G:\APOLLO\DATA\211117\1117095.D Vial: 95  
 Acq On : 11-19-21 5:50:21 Operator: KA  
 Sample : 211116A BLK 5/1000 SG Inst : Apollo  
 Misc : water Multiplr: 5.00  
 IntFile : events.e  
 Quant Time: Nov 19 18:48 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Nov 18 13:26:01 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A

Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.42	174081907	139.154 ppb
Surrogate Spike 150.000		Recovery =	92.77%
4) SA Octacosane(S)	9.65	158850860	175.609 ppb
Surrogate Spike 150.000		Recovery =	117.07%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	35745855	35.509 ppb
2) HBTM Motor Oil (C24-C40)	14.96	207302374	255.216 ppb



Target Compounds



Quantitation Report

Data File: G:\APOLLO\DATA\211117\1117095.D

Sample : 211116A BLK 5/1000 SG



Quantitation Report (QT Reviewed)

Data File : G:\APOLLO\DATA\211117\1117096.D Vial: 96  
 Acq On : 11-19-21 6:18:24 Operator: KA  
 Sample : 211116A LCS-1 5/1000 SG Inst : Apollo  
 Misc : water Multiplr: 5.00  
 IntFile : events.e  
 Quant Time: Nov 19 18:48 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Nov 18 13:26:01 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A

Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.42	210021360	167.882 ppb
Surrogate Spike 150.000		Recovery =	111.92%
4) SA Octacosane(S)	9.66	168568257	186.352 ppb
Surrogate Spike 150.000		Recovery =	124.23%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	2317927612	2302.575 ppb
2) HBTM Motor Oil (C24-C40)	14.96	1701312018	2457.566 ppb
Target Compounds			



Diesel:

$$\frac{(2317927612)(5)}{(2516669)(2)} = \frac{1.16 \times 10^{10}}{5033338} = \boxed{2302.575}$$

Quantitation Report

Data File: G:\APOLLO\DATA\211117\1117096.D

Sample : 211116A LCS-1 5/1000 SG



Data File : G:\APOLLO\DATA\211117\1117097.D Vial: 97  
 Acq On : 11-19-21 6:46:28 Operator: KA  
 Sample : 211116A LCSD-1 5/1000 SG Inst : Apollo  
 Misc : water Multiplr: 5.00  
 IntFile : events.e  
 Quant Time: Nov 19 18:49 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Nov 18 13:26:01 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A



Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.42	179035250	143.113 ppb
Surrogate Spike 150.000		Recovery =	95.41%
4) SA Octacosane(S)	9.66	151052759	166.988 ppb
Surrogate Spike 150.000		Recovery =	111.33%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	1953987014	1941.045 ppb
2) HBTM Motor Oil (C24-C40)	14.96	1539526870	2219.076 ppb

Target Compounds

Quantitation Report

Data File: G:\APOLLO\DATA\211117\1117097.D

Sample : 211116A LCSD-1 5/1000 SG



**Diesel / Motor Oil Calibration Curve**

**Prepared: 10/28/2021**

**Expires: 5/31/2026**

**Prepared By (Initials): KA**

**Methylene**

**e**

**Chloride**

**Lot No. 61117**

Initial Standard Information							Final Standard			
Name of Initial Standard (QAU Label)	Supplier	Conc. (ug/mL)	APPL Mix Name	Reference to APPL Prep Date and Lot #'s	Exp. Date	Exp. Date (Manufacturer)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/mL)
Diesel / Motor Oil - 2	APPL	10	Diesel / Motor Oil - 1	Perp'd: 10/6/21 A0164485-52822, A0168842-52820, A0166510-52817 CL16893-52835	See man. Exp date	10/31/2027 12/31/2027 5/31/2026	100uL	200uL	MC	5
Diesel / Motor Oil - 3		50	Diesel / Motor Oil - 2				200uL	1mL	MC	10
Diesel / Motor Oil Calibration STD	Restek	2,000	Diesel / Motor Oil - 3				25uL	1mL	MC	50
			Diesel / Motor Oil - 4				125uL	1mL	MC	250
			Diesel / Motor Oil - 5				500uL	1mL	MC	1000
			Diesel / Motor Oil - 6				750uL	1mL	MC	1500
			Diesel / Motor Oil - 7				100uL	100uL	N/A	2,000

**Diesel / Motor Oil Second Source**

**Prepared: 10/28/2021**

**Expires: 10/28/2024**

**Prepared By (Initials): KA**

**Methylen**

**e**

**Chloride**

**Lot No. 61117**

Initial Standard Information							Final Standard			
Name of Initial Standard (QAU Label)	Supplier	Supplier Part No.	Conc. (ug/mL)	Lot Number - QA Number	Exp. Date (1 yr.)	Exp. Date (Manufacturer)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/mL)
Diesel Fuel #2 Second Source	Phenova	ALO-101287	50,000	CL16477-52980	See man. Exp date	2/28/2027	50uL	10mL	MC	250
Motor Oil Second Source	Absolute	51094	50,000	102819-52981		10/28/2024	50uL			

**Diesel / Motor Oil CCV**

Prepared: 10/27/2021

Expires: 5/31/2026

Prepared By (Initials): KA

Methylen

e

Chloride

Lot No. 61117

Initial Standard Information							Final Standard			
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference to APPL Prep Date and Lot #'s	Exp. Date	Exp. Date (Manufacturer)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/mL)
Diesel / Motor Oil STD	Restek	Diesel / Motor Oil CCV	2,000	Perp'd: 10/06/21 A0164485-52822, A0168842-52820, A0166510-52817, CL16893-52835	<b>See man. Exp date</b>	10/31/2027 12/31/2027 5/31/2026	1250uL	10mL	MC	250



**Diesel Motor Oil Mix**

Prepared: 10/30/2021

Prepared By (Initials): KA

Expires: 10/31/2027

Initial Standard Information							Final Standard			
Name of Initial Standard (QAU Label)	Supplier	Supplier Part No.	Conc. (ug/mL)	Lot Number - QA Number	Exp. Date (1 yr.)	Exp. Date (Manufacturer)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/mL)
Diesel Fuel #2	Restek	31258	50,000	A0164485-52825 and A0164586-53175, 53174, and 53176	See man. Date	10/31/2027	4.00 mL	8.0 mL	NA	25,000
Motor Oil Composite	Restek	31464	50,000	A0166510-52817, and A0168842-53169, 53170, and 53171	See man. Date	12/31/2027 3/31/28	4.00 mL			25,000

**THC Surrogate**

Prepared: 11/10/2021

KA

Expires: 5/31/2026

Initial Standard Information							Final Standard			
Name of Initial Standard (QAU Label)	Supplier	Supplier Part No.	Conc. (ug/mL)	Lot Number - QA Number	Exp. Date (1 yr.)	Exp. Date (Manufacturer)	Allquot From Stock	Final Volume	Solvent	Final Standard Conc (ug/mL)
O-terphenyl / Octacosane Mix	Phenova	ALO-130161	600	CL16893-52839	See man. Date	5/31/2026	N/A	N/A	N/A	600

**Decanoic Acid Calibration Curve**

Prepared: 9/11/2021

Prepared By (Initials): KA

Expires: 7/12/2022

Methylene

e

Chloride

Lot No. 61117

Initial Standard Information							Final Standard			
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturer)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/mL)
Decanoic Acid STD	O2SI	Decanoic Acid-1	60	Prepared 9/11/21	7/12/2022	N/A	50uL	1mL	MC	3
		Decanoic Acid-2					100uL	1mL	MC	6
		Decanoic Acid-3					400uL	1mL	MC	24
		Decanoic Acid-4					600uL	1mL	MC	36
		Decanoic Acid-5					800uL	1mL	MC	48
		Decanoic Acid-6					100uL	100uL	N/A	60

**Decanoic Acid CCV**

Prepared: 11/5/2021

Prepared By (Initials): KA

Expires: 7/8/2024

Methylene

e

Chloride

Lot No. 61117

Initial Standard Information							Final Standard Information			
Name of Initial Standard (QAU Label)	Supplier	Supplier Part No.	Conc. (ug/mL)	Lot Number - QA Number	Exp. Date	Exp. Date (Manufacturer)	Allquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/mL)
Decanoic Acid	O2SI	72766	1,000	070821-52989	See man. Exp date	7/8/2024	360uL	10mL	MC	36

**Decanoic Acid Spike**

Prepared: 11/5/2021

Prepared By (Initials): KA

Expires: 7/8/2024

Initial Standard Information							Final Standard Information			
Name of Initial Standard (QAU Label)	Supplier	Supplier Part No.	Conc. (ug/mL)	Lot Number - QA Number	Exp. Date (1 yr.)	Exp. Date (Manufacturer)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/mL)
Decanoic Acid Spike	Absolute	72766	1,000	070821-52990	See man. Exp date	7/8/2024	N/A	N/A	N/A	1,000

# Organic Extraction Worksheet

<b>Method</b>	Continuous Liq/Liq TPH- 3520C w/SGC	<b>Extraction Set</b>	211116A	<b>Extraction Method</b>	LIQ005SGC	<b>Units</b>	mL
Spiked ID 1	Diesel Motor Oil Mix 10-30-21 10-31-27	Surrogate ID 1	THC Surrogate 11-10-21 11-10-22				
Spiked ID 2	Decanoic 1000ug/mL Acid Solution 11-5-21 11-5-22	Surrogate ID 2					
Spiked ID 3		Surrogate ID 3					
Spiked ID 4		Surrogate ID 4					
Spiked ID 5		Surrogate ID 5					
Spiked ID 6		Sufficient Vol for Matrix QC:		NO			
Spiked ID 7		Ext. Start Time:	11/16/21 13:42				
Spiked ID 8		Ext. End Time:	11/17/21 7:48				
		<b>GC Requires Extract By:</b>					
pH1	2	11/16/21 12:10	Water Bath Temp 1 °C	35/34.1 °C			
pH2			Water Bath Temp 2 °C	35/36.1			
pH3			Water Bath Temp 3 °C	35/35.5 °C			

Spiked By: SR

Date 11/16/2021

Witnessed By: CG

Date 11/16/2021

Sample	Sample Container	Spike Amount	Spike ID	Surrogate Amount	Surrogate ID	Extract Amount	Final Volume	pH	Extract Date/Time	Comments
121116A Blk		0.050	2	0.250	1	1000	5	2	11/16/21 12:12	*
					equip	E-HP3 E-WB1				
221116A LCS-1		0.080,0.050	1,2	0.250	1	1000	5	2	11/16/21 12:12	*
					equip	E-HP4 E-WB2				
321116A LCSD-1		0.080,0.050	1,2	0.250	1	1000	5	2	11/16/21 12:12	*
					equip	E-HP6 E-WB3				
4BA46001	BA46001W09	0.050	2	0.250	1	1020	5	2	11/16/21 12:12	98213 *
					equip	E-HP7 E-WB1				
5BA46103	BA46103W09	0.050	2	0.250	1	1020	5	2	11/16/21 12:12	98214 *
					equip	E-HP8 E-WB2				
6BA46105	BA46105W09	0.050	2	0.250	1	1040	5	2	11/16/21 12:12	98214 *
					equip	E-HP9 E-WB3				
7BA46107	BA46107W09	0.050	2	0.250	1	1050	5	2	11/16/21 12:12	98214 *
					equip	E-HP10 E-WB1				
8BA46109	BA46109W09	0.050	2	0.250	1	1010	5	2	11/16/21 12:12	98214 *
					equip	E-HP11 E-WB2				
9BA46115	BA46115W09	0.050	2	0.250	1	1040	5	2	11/16/21 12:12	98212 *
					equip	E-HP12 E-WB3				
10BA46116	BA46116W07	0.050	2	0.250	1	1020	5	2	11/16/21 12:12	98212 *
					equip	E-HP13 E-WB1				
11BA46117	BA46117W03	0.050	2	0.250	1	1020	5	2	11/16/21 12:12	98212 *
					equip	E-HP14 E-WB2				

Solvent and Lot#	
1+1 HCL (5mLs)	60358
PH Strips	HC155968
Dichloromethane (DCM)	61117
Filter Paper	400202
Sodium Sulfate	2021071206
SILICA GEL (*)	050627T

Extraction COC Transfer	
Extraction lab employee Initials	KY
GC analyst's initials	KA
Date	11/18/21
Time	10:48
Refrigerator	HOBART

Technician's Initials	
Scanned By	SR
Sample Preparation	SR
Extraction	SR
Concentration	SR,DS

Modified 11/18/2021 7:17:39 AM

Reviewed By: KY

Date 11/18/2021

## Injection Log

Directory: G:\APOLLO\DATA\210911\

Line	Vial	FileName	Multiplier	SampleName	Misc Info	Injected
1	2	911002.D	1	Decanoic Acid STD 1	water	9-11-21 10:22:53
2	3	911003.D	1	Decanoic Acid STD 2	water	9-11-21 10:51:11
3	4	911004.D	1	Decanoic Acid STD 3	water	9-11-21 11:19:39
4	5	911005.D	1	Decanoic Acid STD 4	water	9-11-21 11:48:04
5	6	911006.D	1	Decanoic Acid STD 5	water	9-11-21 12:16:37
6	7	911007.D	1	Decanoic Acid STD 6	water	9-11-21 12:45:02
7	3	1028003.D	1	DMO STD 1 10/28/21	water	10-28-21 9:19:03
8	4	1028004.D	1	DMO STD 2 10/28/21	water	10-28-21 9:47:06
9	5	1028005.D	1	DMO STD 3 10/28/21	water	10-28-21 10:15:13
10	6	1028006.D	1	DMO STD 4 10/28/21	water	10-28-21 10:43:31
11	7	1028007.D	1	DMO STD 5 10/28/21	water	10-28-21 11:11:42
12	8	1028008.D	1	DMO STD 6 10/28/21	water	10-28-21 11:39:55
13	9	1028009.D	1	DMO STD 7 10/28/21	water	10-28-21 12:08:10
14	10	1028010.D	1	DMO Second Source 10/28/21	water	10-28-21 12:36:26
15	92	1117092.D	1	DMO LVL 4 CCV 10/27/21	water	11-19-21 4:26:09
16	93	1117093.D	1	Decanoic Acid CCV 11/05/21	water	11-19-21 4:54:12
17	95	1117095.D	5	211116A BLK 5/1000 SG	water	11-19-21 5:50:21
18	96	1117096.D	5	211116A LCS-1 5/1000 SG	water	11-19-21 6:18:24
19	97	1117097.D	5	211116A LCSD-1 5/1000 SG	water	11-19-21 6:46:28
20	3	1117103.D	4.80769	BA46115W09 5/1040 SG	water	11-19-21 9:34:44
21	4	1117104.D	4.90196	BA46116W07 5/1020 SG	water	11-19-21 10:02:48
22	5	1117105.D	4.90196	BA46117W03 5/1020 SG	water	11-19-21 10:30:53
23	6	1117106.D	1	DMO LVL 4 CCV 10/27/21	water	11-19-21 10:58:57
24	7	1117107.D	1	Decanoic Acid CCV 11/05/21	water	11-19-21 11:26:58

**ORGANICS**  
**Calibration Data**



TPH Extractables  
DOC1028

Form 6  
Initial Calibration

Lab Name: APPL, Inc. \_\_\_\_\_

SDG No: \_\_\_\_\_

Case No: \_\_\_\_\_

Initial Cal. Date: 10/28/2021 \_\_\_\_\_

Matrix: Water \_\_\_\_\_

Instrument: Apollo \_\_\_\_\_

Initials: KA \_\_\_\_\_

1028003.D    1028004.D    1028005.D    1028006.D    1028007.D    1028008.D    1028009.D

	Compound	1	2	3	4	5	6	7				Avg	%RSD	Type	r <sup>2</sup>	Q
1	HATM Diesel (C10-C24)	2983809	2406563	2517872	2418941	2337993	2387715	2563791				2516669	8.7	HATM		
2	HBTML Motor Oil (C24-C40)	5192328	3260715	2065863	1824592	1695984	1676117	1728658				2492037	53	HBTM	1.000	
3	SA Ortho-Terphenyl(S)	3637234	3178668	3119876	3035678	2926966	2905323	3088794				3127505	7.9	SA		
4	SA Octacosane(S)	2469203	2170507	2286410	2275552	2170413	2171254	2286658				2261428	4.8	SA		
5																
6																
7																
8																
9																
10																
11																
12																
13																
14																
15																
16																
17																
18																
19																
20																
21																
22																
23																
24																
25																
26																
27																
28																
29																
30																
31																
32																
33																
34																
35																

2.118919

Data File : G:\APOLLO\DATA\211028\1028003.D Vial: 3  
 Acq On : 10-28-21 9:19:03 Operator: KA  
 Sample : DMO STD 1 10/28/21 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Oct 28 15:39 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Oct 28 15:39:11 2021  
 Response via : Multiple Level Calibration




Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A

Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.53	1818617	0.291 ppb
Surrogate Spike 30.000		Recovery =	0.97%
4) SA Octacosane(S)	9.82	1234601	0.273 ppb
Surrogate Spike 30.000		Recovery =	0.91%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	29838086	5.928 ppb
2) HBTM Motor Oil (C24-C40)	14.96	51923283	5.234 ppb
Target Compounds			

Quantitation Report

Data File: G:\APOLLO\DATA\211028\1028003.D

Sample : DMO STD 1 10/28/21



Data File : G:\APOLLO\DATA\211028\1028004.D Vial: 4  
 Acq On : 10-28-21 9:47:06 Operator: KA  
 Sample : DMO STD 2 10/28/21 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Oct 28 15:39 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Oct 28 15:39:11 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A




Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.53	3178668	0.508 ppb
Surrogate Spike 30.000		Recovery =	1.69%
4) SA Octacosane(S)	9.82	2170507	0.480 ppb
Surrogate Spike 30.000		Recovery =	1.60%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	48131263	9.562 ppb
2) HBTM Motor Oil (C24-C40)	14.96	65214303	9.152 ppb

Target Compounds

Quantitation Report

Data File: G:\APOLLO\DATA\211028\1028004.D

Sample : DMO STD 2 10/28/21



Data File : G:\APOLLO\DATA\211028\1028005.D Vial: 5  
 Acq On : 10-28-21 10:15:13 Operator: KA  
 Sample : DMO STD 3 10/28/21 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Oct 28 15:39 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Oct 28 15:39:11 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A




Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.53	15599382	2.494 ppb
Surrogate Spike 30.000		Recovery =	8.31%
4) SA Octacosane(S)	9.82	11432050	2.528 ppb
Surrogate Spike 30.000		Recovery =	8.43%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	251787231	50.024 ppb
2) HBTM Motor Oil (C24-C40)	14.96	206586322	50.832 ppb

Target Compounds

Quantitation Report

Data File: G:\APOLLO\DATA\211028\1028005.D

Sample : DMO STD 3 10/28/21



Quantitation Report (Not Reviewed)

Data File : G:\APOLLO\DATA\211028\1028006.D Vial: 6  
 Acq On : 10-28-21 10:43:31 Operator: KA  
 Sample : DMO STD 4 10/28/21 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Oct 28 15:39 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Oct 28 15:39:11 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A



Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.53	75891940	12.133 ppb
Surrogate Spike 30.000		Recovery =	40.44%
4) SA Octacosane(S)	9.82	56888797	12.578 ppb
Surrogate Spike 30.000		Recovery =	41.93%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	1209470396	240.292 ppb
2) HBTM Motor Oil (C24-C40)	14.96	912296132	258.892 ppb
Target Compounds			



Quantitation Report

Data File: G:\APOLLO\DATA\211028\1028006.D

Sample : DMO STD 4 10/28/21



Quantitation Report (Not Reviewed)

Data File : G:\APOLLO\DATA\211028\1028007.D Vial: 7  
 Acq On : 10-28-21 11:11:42 Operator: KA  
 Sample : DMO STD 5 10/28/21 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Oct 28 15:39 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Oct 28 15:39:11 2021  
 Response via : Multiple Level Calibration



Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A

Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.54	292696553	46.794 ppb
Surrogate Spike 30.000		Recovery =	155.98%
4) SA Octacosane(S)	9.83	217041298	47.988 ppb
Surrogate Spike 30.000		Recovery =	159.96%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	4675985227	929.003 ppb
2) HBTM Motor Oil (C24-C40)	14.96	3391967397	989.959 ppb

Target Compounds

Quantitation Report

Data File: G:\APOLLO\DATA\211028\1028007.D  
Sample : DMO STD 5 10/28/21



Data File : G:\APOLLO\DATA\211028\1028008.D Vial: 8  
 Acq On : 10-28-21 11:39:55 Operator: KA  
 Sample : DMO STD 6 10/28/21 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Oct 28 15:39 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Oct 28 15:39:11 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A



Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.54	435798382	69.672 ppb
Surrogate Spike 30.000		Recovery =	232.24%
4) SA Octacosane(S)	9.84	325688048	72.009 ppb
Surrogate Spike 30.000		Recovery =	240.03%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	7163144090	1423.140 ppb
2) HBTM Motor Oil (C24-C40)	14.96	5028351305	1472.405 ppb

Target Compounds

Quantitation Report

Data File: G:\APOLLO\DATA\211028\1028008.D

Sample : DMO STD 6 10/28/21



Data File : G:\APOLLO\DATA\211028\1028009.D Vial: 9  
 Acq On : 10-28-21 12:08:10 Operator: KA  
 Sample : DMO STD 7 10/28/21 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Oct 28 15:39 2021 Quant Results File: DOC1028.RES



Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Oct 28 15:39:11 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A

Compound	R.T.	Response	Conc Units
-----			
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.54	617758709	98.762 ppb
Surrogate Spike 30.000		Recovery =	329.21%
4) SA Octacosane(S)	9.85	457331573	101.116 ppb
Surrogate Spike 30.000		Recovery =	337.05%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	10255165539	2037.448 ppb
2) HBTM Motor Oil (C24-C40)	14.96	6914631831	2028.526 ppb
Target Compounds			

Quantitation Report

Data File: G:\APOLLO\DATA\211028\1028009.D  
Sample : DMO STD 7 10/28/21



TPH Extractables  
DOC1028

Form 7

Second Source Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Date Analyzed: 10/28/2021  
Instrument: Apollo  
Initial Cal. Date: 10/28/2021  
Data File: 1028010.D

	Compound	MEAN	CCRF	%D	%Drift
1	HATM Diesel (C10-C24)	2516670	2266400	9.9	HATM
2	HBTM Motor Oil (C24-C40)	2492040	1663520	33	HBTML 5.9
3					
4					
5					
6					
7					
8					
9					
10					
11					
12					
13					
14					
15					
16					
17					
18					
19					
20					
21					
22					
23					
24					
25					
26					
27					
28					
29					
30					
31					
32					
33					
34					
35					
36					
37					
38					
39					
40	Average			21.5	



Data File : G:\APOLLO\DATA\211028\1028010.D Vial: 10  
 Acq On : 10-28-21 12:36:26 Operator: KA  
 Sample : DMO Second Source 10/28/21 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Oct 28 15:39 2021 Quant Results File: DOC1028.RES



Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Oct 28 15:39:11 2021  
 Response via : Multiple Level Calibration


Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A

Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.53	4250105	0.679 ppb
Surrogate Spike 30.000		Recovery =	2.26%
4) SA Octacosane(S)	9.83	-3553	N.D. ppb
Surrogate Spike 30.000		Recovery =	0.00%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	1133202337	225.139 ppb
2) HBTM Motor Oil (C24-C40)	14.96	831758038	235.148 ppb
Target Compounds			

Quantitation Report

Data File: G:\APOLLO\DATA\211028\1028010.D  
Sample : DMO Second Source 10/28/21





Method Name: G:\APOLLO\DATA\211028\DOC1028.M  
 Calibration Table Last Updated: Thu Oct 28 15:37:06 2021

TPH Extractables  
DOC1028

Form 7

Continuing Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Date Analyzed: 11/17/2021  
Instrument: Apollo  
Initial Cal. Date: 10/28/2021  
Data File: 1117025.D

	Compound	MEAN	CCRF	%D	%Drift
1	HATM Diesel (C10-C24)	2516670	2674370	6.3	HATM
2	HBTM Motor Oil (C24-C40)	2492040	1913490	23	HBTML 8.8
3	SA Ortho-Terphenyl(S)	3127510	3232370	3.4	SA
4	SA Octacosane(S)	2261430	2381760	5.3	SA
5					
6					
7					
8					
9					
10					
11					
12					
13					
14					
15					
16					
17					
18					
19					
20					
21					
22					
23					
24					
25					
26					
27					
28					
29					
30					
31					
32					
33					
34					
35					
36					
37					
38					
39					
40	Average			9.5	

Quantitation Report (Not Reviewed)

Data File : G:\APOLLO\DATA\211117\1117025.D Vial: 25  
 Acq On : 11-17-21 21:03:23 Operator: KA  
 Sample : DMO LVL 4 CCV 10/27/21 Inst : Apollo  
 Misc : Water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Nov 19 10:17 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Nov 18 13:26:01 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A



Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.43	80809311	12.919 ppb
Surrogate Spike 30.000		Recovery =	43.06%
4) SA Octacosane(S)	9.67	59544117	13.165 ppb
Surrogate Spike 30.000		Recovery =	43.88%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	1337183531	265.665 ppb
2) HBTM Motor Oil (C24-C40)	14.96	956746034	271.997 ppb

Target Compounds

Quantitation Report

Data File: G:\APOLLO\DATA\211117\1117025.D

Sample : DMO LVL 4 CCV 10/27/21



TPH Extractables  
DOC1028

Form 7

Continuing Calibration

Lab Name: APPL, Inc.

SDG No: \_\_\_\_\_

Case No: \_\_\_\_\_

Date Analyzed: 11/18/2021

Matrix: Water

Instrument: Apollo

Initial Cal. Date: 10/28/2021

Data File: 1117039.D

		Compound	MEAN	CCRF	%D		%Drift
1	HATM	Diesel (C10-C24)	2516670	2736840	8.7	HATM	
2	HBTM	Motor Oil (C24-C40)	2492040	1943430	22	HBTML	11
3	SA	Ortho-Terphenyl(S)	3127510	3295850	5.4	SA	
4	SA	Octacosane(S)	2261430	2449290	8.3	SA	
5							
6							
7							
8							
9							
10							
11							
12							
13							
14							
15							
16							
17							
18							
19							
20							
21							
22							
23							
24							
25							
26							
27							
28							
29							
30							
31							
32							
33							
34							
35							
36							
37							
38							
39							
40							

Average

11.1

Data File : G:\APOLLO\DATA\211117\1117039.D Vial: 39  
 Acq On : 11-18-21 3:36:02 Operator: KA  
 Sample : DMO LVL 4 CCV 10/27/21 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Nov 19 10:15 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Nov 18 13:26:01 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A

Compound	R.T.	Response	Conc Units
<b>System Monitoring Compounds</b>			
3) SA Ortho-Terphenyl(S)	7.43	82396154	13.173 ppb
Surrogate Spike 30.000		Recovery =	43.91%
4) SA Octacosane(S)	9.66	61232212	13.538 ppb
Surrogate Spike 30.000		Recovery =	45.13%
<b>Target Compounds</b>			
1) HATM Diesel (C10-C24)	6.49	1368421302	271.872 ppb
2) HBTM Motor Oil (C24-C40)	14.96	971713672	276.410 ppb



Target Compounds



Quantitation Report

Data File: G:\APOLLO\DATA\211117\1117039.D

Sample : DMO LVL 4 CCV 10/27/21



TPH Extractables  
DOC1028

Form 7  
Continuing Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Date Analyzed: 11/18/2021  
Instrument: Apollo  
Initial Cal. Date: 10/28/2021  
Data File: 1117056.D

		Compound	MEAN	CCRF	%D	%Drift	
1	HATM	Diesel (C10-C24)	2516670	2802350	11	HATM	
2	HBTM	Motor Oil (C24-C40)	2492040	1987120	20	HBTML	13
3	SA	Ortho-Terphenyl(S)	3127510	3392810	8.5	SA	
4	SA	Octacosane(S)	2261430	2443600	8.1	SA	
5							
6							
7							
8							
9							
10							
11							
12							
13							
14							
15							
16							
17							
18							
19							
20							
21							
22							
23							
24							
25							
26							
27							
28							
29							
30							
31							
32							
33							
34							
35							
36							
37							
38							
39							
40							

Average

11.9

Data File : G:\APOLLO\DATA\211117\1117056.D Vial: 56  
 Acq On : 11-18-21 11:32:57 Operator: KA  
 Sample : DMO LVL 4 CCV 10/27/21 Inst : Apollo  
 Misc : water Multiplr: 1.00  
 IntFile : events.e  
 Quant Time: Nov 19 10:21 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Nov 18 13:26:01 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A



Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.43	84820246	13.560 ppb
Surrogate Spike 30.000		Recovery =	45.20%
4) SA Octacosane(S)	9.66	61090101	13.507 ppb
Surrogate Spike 30.000		Recovery =	45.02%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	1401173186	278.379 ppb
2) HBTM Motor Oil (C24-C40)	14.96	993561842	282.851 ppb

Target Compounds:

Quantitation Report

Data File: G:\APOLLO\DATA\211117\1117056.D

Sample : DMO LVL 4 CCV 10/27/21



**ORGANICS**  
**Raw Data**

Data File : G:\APOLLO\DATA\211117\1117037.D Vial: 37  
 Acq On : 11-18-21 2:39:54 Operator: KA  
 Sample : BA46118W01 5/1000 Inst : Apollo  
 Misc : water Multiplr: 5.00  
 IntFile : events.e  
 Quant Time: Nov 19 13:08 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Nov 18 13:26:01 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A



Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.43	94982315	75.925 ppb
Surrogate Spike 150.000		Recovery =	50.62%
4) SA Octacosane(S)	9.66	84783721	93.728 ppb
Surrogate Spike 150.000		Recovery =	62.49%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	28359583	28.172 ppb
2) HBTM Motor Oil (C24-C40)	14.96	63400001	43.087 ppb

Target Compounds

Quantitation Report

Data File: G:\APOLLO\DATA\211117\1117037.D

Sample : BA46118W01 5/1000



Data File : G:\APOLLO\DATA\211117\1117038.D Vial: 38  
 Acq On : 11-18-21 3:08:00 Operator: KA  
 Sample : BA46119W01 5/1000 Inst : Apollo  
 Misc : water Multiplr: 5.00  
 IntFile : events.e  
 Quant Time: Nov 19 13:09 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Nov 18 13:26:01 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A



Compound	R.T.	Response	Conc Units
<b>System Monitoring Compounds</b>			
3) SA Ortho-Terphenyl(S)	7.43	132867950	106.209 ppb
Surrogate Spike 150.000		Recovery =	70.81%
4) SA Octacosane(S)	9.66	119896941	132.546 ppb
Surrogate Spike 150.000		Recovery =	88.36%
<b>Target Compounds</b>			
1) HATM Diesel (C10-C24)	6.49	48322528	48.002 ppb
2) HBTM Motor Oil (C24-C40)	14.96	66514229	47.677 ppb
<b>Target Compounds</b>			



Quantitation Report

Data File: G:\APOLLO\DATA\211117\1117038.D

Sample : BA46119W01 5/1000



Data File : G:\APOLLO\DATA\211117\1117029.D Vial: 29  
 Acq On : 11-17-21 22:55:31 Operator: KA  
 Sample : 211115A BLK 5/1000 Inst : Apollo  
 Misc : water Multiplr: 5.00  
 IntFile : events.e  
 Quant Time: Nov 19 13:04 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Nov 18 13:26:01 2021  
 Response via : Multiple Level Calibration



Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A

Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.43	129864089	103.808 ppb
Surrogate Spike 150.000		Recovery =	69.21%
4) SA Octacosane(S)	9.67	118110389	130.571 ppb
Surrogate Spike 150.000		Recovery =	87.05%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	43387000	43.100 ppb
2) HBTM Motor Oil (C24-C40)	14.96	54832278	30.457 ppb

Target Compounds

Data File: G:\APOLLO\DATA\211117\1117029.D

Sample : 211115A BLK 5/1000



Data File : G:\APOLLO\DATA\211117\1117030.D Vial: 30  
 Acq On : 11-17-21 23:23:35 Operator: KA  
 Sample : 211115A LCS-1 5/1000 Inst : Apollo  
 Misc : water Multiplr: 5.00  
 IntFile : events.e  
 Quant Time: Nov 19 13:05 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Nov 18 13:26:01 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A

Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.43	132417916	105.849 ppb
Surrogate Spike 150.000		Recovery =	70.57%
4) SA Octacosane(S)	9.66	119590605	132.207 ppb
Surrogate Spike 150.000		Recovery =	88.14%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	46085413	45.780 ppb
2) HBTM Motor Oil (C24-C40)	14.96	65228159	45.782 ppb
Target Compounds			



Diesel :

$$\frac{(46085413)(5)}{(2516669)(2)} = \frac{230427065}{5033338} = \boxed{45.780}$$

Quantitation Report

Data File: G:\APOLLO\DATA\211117\1117030.D

Sample : 211115A LCS-1 5/1000



Data File : G:\APOLLO\DATA\211117\1117031.D Vial: 31  
 Acq On : 11-17-21 23:51:36 Operator: KA  
 Sample : 211115A LCSD-1 5/1000 Inst : Apollo  
 Misc : water Multiplr: 5.00  
 IntFile : events.e  
 Quant Time: Nov 19 13:06 2021 Quant Results File: DOC1028.RES

Method : G:\APOLLO\DATA\211028\DOC1028.M (Chemstation Integrator)  
 Title : 8015 B&C  
 Last Update : Thu Nov 18 13:26:01 2021  
 Response via : Multiple Level Calibration

Volume Inj. : 2UL  
 Signal Phase : DB-5  
 Signal Info : FID02A



Compound	R.T.	Response	Conc Units
System Monitoring Compounds			
3) SA Ortho-Terphenyl(S)	7.43	126568035	101.173 ppb
Surrogate Spike 150.000		Recovery =	67.45%
4) SA Octacosane(S)	9.66	114275506	126.331 ppb
Surrogate Spike 150.000		Recovery =	84.22%
Target Compounds			
1) HATM Diesel (C10-C24)	6.49	46367651	46.061 ppb
2) HBTM Motor Oil (C24-C40)	14.96	67756669	49.509 ppb

Target Compounds

Quantitation Report

Data File: G:\APOLLO\DATA\211117\1117031.D

Sample : 211115A LCSD-1 5/1000



## Diesel / Motor Oil Calibration Curve

Prepared: 10/28/2021

Expires: 5/31/2026

Prepared By (Initials): KA

Methylen

e

Chloride

Lot No. 61117

Initial Standard Information							Final Standard			
Name of Initial Standard (QAU Label)	Supplier	Conc. (ug/mL)	APPL Mix Name	Reference to APPL Prep Date and Lot #'s	Exp. Date	Exp. Date (Manufacturer)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/mL)
Diesel / Motor Oil - 2	APPL	10	Diesel / Motor Oil - 1	Prep'd: 10/8/21 A0164485-82822, A0168842-52820, AO166510-52817 CL16893-52835	See man. Exp date	10/31/2027 12/31/2027 5/31/2026	100uL	200uL	MC	5
Diesel / Motor Oil - 3		50	Diesel / Motor Oil - 2				200uL	1mL	MC	10
Diesel / Motor Oil Calibration STD	Restek	2,000	Diesel / Motor Oil - 3				25uL	1mL	MC	50
			Diesel / Motor Oil - 4				125uL	1mL	MC	250
			Diesel / Motor Oil - 5				500uL	1mL	MC	1000
			Diesel / Motor Oil - 6				750uL	1mL	MC	1500
			Diesel / Motor Oil - 7				100uL	100uL	N/A	2,000



**Diesel / Motor Oil Second Source**

**Prepared: 10/28/2021**

**Expires: 10/28/2024**

**Prepared By (Initials): KA**

**Methylen**

**e**

**Chloride**

**Lot No. 61117**

Initial Standard Information							Final Standard			
Name of Initial Standard (QAU Label)	Supplier	Supplier Part No.	Conc. (ug/mL)	Lot Number - QA Number	Exp. Date (1 yr.)	Exp. Date (Manufacturer)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/mL)
Diesel Fuel #2 Second Source	Phenova	ALO-101287	50,000	CL16477-52980	See man. Exp date	2/28/2027	50uL	10mL	MC	250
Motor Oil Second Source	Absolute	51094	50,000	102819-52981		10/28/2024	50uL			

**Diesel / Motor Oil CCV**

Prepared: 10/27/2021

Expires: 5/31/2026

Prepared By (Initials): KA

Methylen

e

Chloride

Lot No. 61117

Initial Standard Information							Final Standard			
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference to APPL Prep Date and Lot #'s	Exp. Date	Exp. Date (Manufacturer)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/mL)
Diesel / Motor Oil STD	Restek	Diesel / Motor Oil CCV	2,000	Perp'd: 10/06/21 A0164485-52822, A0168842-52820, A0166510-52817, CL16893-52835	<b>See man. Exp date</b>	10/31/2027 12/31/2027 5/31/2026	1250uL	10mL	MC	250

THC Surrogate										
Prepared: 11/10/2021							KA			
Expires: 5/31/2026										
Initial Standard Information							Final Standard			
Name of Initial Standard (QAU Label)	Supplier	Supplier Part No.	Conc. (ug/mL)	Lot Number - QA Number	Exp. Date (1 yr.)	Exp. Date (Manufacturer)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/mL)
O-terphenyl / Octacosane Mix	Phenova	ALO-130161	600	CL16893-52839	See man. Date	5/31/2026	N/A	N/A	N/A	600

# Organic Extraction Worksheet

<b>Method</b>	Continuous Liq/Liq TPH-Diesel/MO 3520C	<b>Extraction Set</b>	211115A	<b>Extraction Method</b>	LIQ005	<b>Units</b>	mL
Spiked ID 1		Surrogate ID 1	THC Surrogate 11-10-21 11-10-22				
Spiked ID 2		Surrogate ID 2					
Spiked ID 3		Surrogate ID 3					
Spiked ID 4		Surrogate ID 4					
Spiked ID 5		Surrogate ID 5					
Spiked ID 6		Sufficient Vol for Matrix QC:		NO			
Spiked ID 7		Ext. Start Time:		11/15/21 13:18			
Spiked ID 8		Ext. End Time:		11/16/21 7:19			
<b>GC Requires Extract By:</b>							
pH1	2	11/15/21 10:15	Water Bath Temp 1 °C	43/42.1 °C			
pH2			Water Bath Temp 2 °C	37/38.1			
pH3			Water Bath Temp 3 °C	35/34.5 °C			

Spiked By: SR

Date 11/15/2021

Witnessed By: CG

Date 11/15/2021

Sample	Sample Container	Spike Amount	Spike ID	Surrogate Amount	Surrogate ID	Extract Amount	Final Volume	pH	Extract Date/Time	Comments
1211115A Blk				0.250	1	1000	5	2	11/15/21 10:19	
					equip	E-HP3 E-WB1				
2211115A LCS-1				0.250	1	1000	5	2	11/15/21 10:19	
					equip	E-HP4 E-WB2				
3211115A LCSD-1				0.250	1	1000	5	2	11/15/21 10:19	
					equip	E-HP6 E-WB3				
4BA46002	BA46002W01			0.250	1	1000	5	2	11/15/21 10:19	98213
					equip	E-HP7 E-WB1				
5BA46110	BA46110W01			0.250	1	1000	5	2	11/15/21 10:19	98214
					equip	E-HP8 E-WB2				
6BA46111	BA46111W01			0.250	1	1000	5	2	11/15/21 10:19	98214
					equip	E-HP9 E-WB1				
7BA46112	BA46112W01			0.250	1	1000	5	2	11/15/21 10:19	98214
					equip	E-HP10 E-WB2				
8BA46113	BA46113W01			0.250	1	1000	5	2	11/15/21 10:19	98214
					equip	E-HP11 E-WB3				
9BA46118	BA46118W01			0.250	1	1000	5	2	11/15/21 10:19	98212
					equip	E-HP12 E-WB1				
10BA46119	BA46119W01			0.250	1	1000	5	2	11/15/21 10:19	98212
					equip	E-HP22 E-WB2				
11BA46120	BA46120W01			0.250	1	1000	5	2	11/15/21 10:19	98212
					equip	E-HP14 E-WB3				

Solvent and Lot#	
1+1 HCL (5mLs)	60358
PH Strips	HC155968
Dicholormethane	61117
Filter Paper	100202
Sodium Sulfate	2021071206

Extraction COC Transfer	
Extraction lab employee Initials	KY
GC analyst's initials	KA
Date	11/17/21
Time	8:24
Refrigerator	Hobart

Technician's Initials	
Scanned By	SR
Sample Preparation	SR
Extraction	SR
Concentration	DS
Modified	11/17/2021 7:15:45 AM

Reviewed By: KY

Date 11/17/2021

## Injection Log

Directory: G:\APOLLO\DATA\211028\

Line	Vial	FileName	Multiplier	SampleName	Misc Info	Injected
1	3	1028003.D	1	DMO STD 1 10/28/21	water	10-28-21 9:19:03
2	4	1028004.D	1	DMO STD 2 10/28/21	water	10-28-21 9:47:06
3	5	1028005.D	1	DMO STD 3 10/28/21	water	10-28-21 10:15:13
4	6	1028006.D	1	DMO STD 4 10/28/21	water	10-28-21 10:43:31
5	7	1028007.D	1	DMO STD 5 10/28/21	water	10-28-21 11:11:42
6	8	1028008.D	1	DMO STD 6 10/28/21	water	10-28-21 11:39:55
7	9	1028009.D	1	DMO STD 7 10/28/21	water	10-28-21 12:08:10
8	10	1028010.D	1	DMO Second Source 10/28/21	water	10-28-21 12:36:26
9	25	1117025.D	1	DMO LVL 4 CCV 10/27/21	Water	11-17-21 21:03:23
10	29	1117029.D	5	211115A BLK 5/1000	water	11-17-21 22:55:31
11	30	1117030.D	5	211115A LCS-1 5/1000	water	11-17-21 23:23:35
12	31	1117031.D	5	211115A LCSD-1 5/1000	water	11-17-21 23:51:36
13	37	1117037.D	5	BA46118W01 5/1000	water	11-18-21 2:39:54
14	38	1117038.D	5	BA46119W01 5/1000	water	11-18-21 3:08:00
15	39	1117039.D	1	DMO LVL 4 CCV 10/27/21	water	11-18-21 3:36:02
16	40	1117040.D	5	BA46120W01 5/1000	water	11-18-21 4:04:05
17	56	1117056.D	1	DMO LVL 4 CCV 10/27/21	water	11-18-21 11:32:57

**ORGANICS**  
**Calibration Data**

PAH by GCMS SIM  
EPA 8270 SIM

Form 6  
Initial Calibration

Lab Name: APPL, Inc.

SDG No: \_\_\_\_\_

Case No: \_\_\_\_\_

Initial Cal. Date: 10/19/2021

Matrix: \_\_\_\_\_

Instrument: KYLO

Initials: LS

1019K002.D 1019K003.D 1019K004.D 1019K005.D 1019K006.D 1019K007.D 1019K008.D 1019K009.D

	Compound	0.1	0.2	0.5	1	5	10	50	100			Avg	%RSD	Type	r <sup>2</sup>	Q	MRF
1	I Naphthalene-D8(IS)																
2	TM Naphthalene	1.428	1.402	1.354	1.336	1.308	1.289	1.172	1.100			1.3	8.6	TM			0.700
3	S 2-Methylnaphthalene-D10 (2M)	1.359	1.337	1.324	1.305	1.316	1.159	1.222	1.192			1.3	5.9	S			
4	TM 2-Methylnaphthalene	0.7868	0.7804	0.7756	0.7764	0.7886	0.7810	0.7175	0.6825			0.76	5.1	TM			0.400
5	TM 1-Methylnaphthalene	0.8005	0.7905	0.7931	0.7961	0.7922	0.7806	0.7122	0.6797			0.77	6.0	TM			
6	I Acenaphthene-D10(IS)																
7	TM Acenaphthylene	5.288	5.373	5.323	5.258	5.439	5.405	4.863	4.456			5.2	6.6	TM			0.900
8	*TM Acenaphthene	1.497	1.444	1.402	1.372	1.398	1.381	1.266	1.207			1.4	6.8	*TM			0.900
9	TM Fluorene	1.615	1.645	1.600	1.590	1.642	1.640	1.521	1.456			1.6	4.2	TM			0.900
10	I Phenanthrene-D10(IS)																
11	TM Phenanthrene	1.510	1.398	1.383	1.377	1.403	1.374	1.309	1.253			1.4	5.4	TM			0.700
12	TM Anthracene	1.298	1.273	1.300	1.300	1.352	1.349	1.285	1.240			1.3	2.8	TM			0.700
13	S Fluoranthene-D10 (FRT)	2.023	1.976	1.895	1.904	2.032	1.918	1.953	1.890			1.9	2.9	S			
14	*TM Fluoranthene	2.169	2.135	2.136	2.147	2.255	2.226	2.086	1.944			2.1	4.4	*TM			0.600
15	I Chrysene-D12(IS)																
16	TM Pyrene	1.986	2.033	1.960	1.958	1.948	1.927	1.782	1.720			1.9	5.6	TM			0.600
17	TM Benz (a) anthracene	1.473	1.441	1.379	1.381	1.401	1.420	1.370	1.344			1.4	3.0	TM			0.800
18	TM Chrysene	1.754	1.672	1.608	1.574	1.554	1.516	1.410	1.375			1.6	8.1	TM			0.700
19	TML Indeno (1,2,3-cd) pyrene	1.687	1.326	1.360	1.404	1.015	1.052	1.169	1.168			1.3	17	TM	1.000		0.500
20	I Perylene-D12(IS)																
21	TM Benzo (b) fluoranthene	1.268	1.292	1.301	1.356	1.511	1.514	1.537	1.485			1.4	8.1	TM			0.700
22	TM Benzo (k) fluoranthene	1.593	1.558	1.636	1.632	1.670	1.730	1.578	1.484			1.6	4.6	TM			0.700
23	*TM Benzo (a) pyrene	1.254	1.223	1.224	1.265	1.442	1.484	1.454	1.383			1.3	8.3	*TM			0.700
24	TM Dibenz (a,h) anthracene	1.360	1.209	1.221	1.273	1.398	1.395	1.399	1.353			1.3	6.0	TM			0.400
25	TM Benzo (g,h,i) perylene	1.457	1.403	1.410	1.405	1.496	1.517	1.462	1.394			1.4	3.2	TM			0.500
26																	
27																	
28																	
29																	
30																	
31																	
32																	
33																	
34																	
35																	

Data File : M:\KYLO\DATA\211019\1019K002.D  
 Acq On : 19 Oct 21 14:09  
 Sample : 0.1 ug/ml 10/13/21  
 Misc :

Vial: 2  
 Operator: LS  
 Inst : KYLO  
 Multiplr: 1.00

Quant Time: Oct 19 15:48 2021

Quant Results File: K1019.RES

Quant Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)  
 Title : EPA 8270  
 Last Update : Tue Oct 19 16:47:23 2021  
 Response via : Initial Calibration  
 DataAcq Meth : SIM\_2

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Napthalene-D8 (IS)	3.92	136	10962	2.50000	ppb	0.00
6) Acenaphthene-D10 (IS)	5.86	164	5295	2.50000	ppb	0.00
10) Phenanthrene-D10 (IS)	7.56	188	8379	2.50000	ppb	0.00
15) Chrysene-D12 (IS)	10.63	240	9693	2.50000	ppb	0.01
20) Perylene-D12 (IS)	12.84	264	9009	2.50000	ppb	0.01

System Monitoring Compounds

3) 2-Methylnaphthalene-D10 (2)	4.66	152	298	0.05323	ppb	0.00
Spiked Amount	5.000		Recovery	=	1.060%	
13) Fluoranthene-D10 (FRT)	8.94	212	339	0.05190	ppb	0.01
Spiked Amount	5.000		Recovery	=	1.040%	

Target Compounds

	R.T.	QIon	Response	Conc	Units	Qvalue
2) Napthalene	3.94	128	626	0.10994	ppb	99
4) 2-Methylnaphthalene	4.69	142	345	0.10338	ppb	100
5) 1-Methylnaphthalene	4.80	142	351	0.10422	ppb	99
7) Acenaphthylene	5.70	152	1120	0.10217	ppb	100
8) Acenaphthene	5.89	154	317	0.10918	ppb	99
9) Fluorene	6.49	166	342	0.10165	ppb	96
11) Phenanthrene	7.59	178	506	0.10973	ppb	100
12) Anthracene	7.65	178	435	0.09988	ppb	97
14) Fluoranthene	8.96	202	727	0.10149	ppb	98
16) Pyrene	9.22	202	770	0.10375	ppb	99
17) Benz (a) anthracene	10.62	228	571	0.10510	ppb	99
18) Chrysene	10.66	228	680	0.11258	ppb	96
19) Indeno (1,2,3-cd) pyrene	14.41	276	654	0.33399	ppb	# 88
22) Benzo (k) fluoranthene	12.21	252	574	-0.45104	ppb	97
23) Benzo (a) pyrene	12.75	252	452	-0.17190	ppb	95
24) Dibenz (a,h) anthracene	14.45	278	490	-0.04905	ppb	95
25) Benzo (g,h,i) perylene	14.71	276	525	-0.23039	ppb	98



Quantitation Report


Data File : M:\KYLO\DATA\211019\1019K002.D  
Acq On : 19 Oct 21 14:09  
Sample : 0.1 ug/ml 10/13/21  
Misc :

Vial: 2  
Operator: LS  
Inst : KYLO  
Multiplr: 1.00

Quant Time: Oct 19 15:48 2021

Quant Results File: K1019.RES

Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)  
Title : EPA 8270  
Last Update : Tue Nov 09 10:14:45 2021  
Response via : Initial Calibration



Data File : M:\KYLO\DATA\211019\1019K003.D  
 Acq On : 19 Oct 21 14:29  
 Sample : 0.2 ug/ml 10/13/21  
 Misc :

Vial: 3  
 Operator: LS  
 Inst : KYLO  
 Multiplr: 1.00

Quant Time: Oct 19 15:48 2021

Quant Results File: K1019.RES

Quant Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)  
 Title : EPA 8270  
 Last Update : Tue Oct 19 16:47:23 2021  
 Response via : Initial Calibration  
 DataAcq Meth : SIM\_2

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Napthalene-D8 (IS)	3.92	136	11180	2.50000	ppb	0.00
6) Acenaphthene-D10 (IS)	5.86	164	5495	2.50000	ppb	0.00
10) Phenanthrene-D10 (IS)	7.56	188	8995	2.50000	ppb	0.00
15) Chrysene-D12 (IS)	10.63	240	9881	2.50000	ppb	0.01
20) Perylene-D12 (IS)	12.84	264	8688	2.50000	ppb	0.01
System Monitoring Compounds						
3) 2-Methylnaphthalene-D10 (2)	4.66	152	598	0.10474	ppb	0.00
Spiked Amount	5.000		Recovery	=	2.100%	
13) Fluoranthene-D10 (FRT)	8.94	212	711	0.10140	ppb	0.01
Spiked Amount	5.000		Recovery	=	2.020%	
Target Compounds						
2) Napthalene	3.94	128	1254	0.21593	ppb	99
4) 2-Methylnaphthalene	4.69	142	698	0.20508	ppb	96
5) 1-Methylnaphthalene	4.80	142	707	0.20582	ppb	98
7) Acenaphthylene	5.69	152	2362	0.20763	ppb	100
8) Acenaphthene	5.89	154	635	0.21074	ppb	99
9) Fluorene	6.49	166	723	0.20706	ppb	100
11) Phenanthrene	7.59	178	1006	0.20323	ppb	100
12) Anthracene	7.65	178	916	0.19592	ppb	99
14) Fluoranthene	8.96	202	1536	0.19974	ppb	97
16) Pyrene	9.21	202	1607	0.21241	ppb	99
17) Benz (a) anthracene	10.62	228	1139	0.20566	ppb	98
18) Chrysene	10.66	228	1322	0.21470	ppb	99
19) Indeno (1,2,3-cd) pyrene	14.40	276	1048	0.41647	ppb	# 98
21) Benzo (b) fluoranthene	12.16	252	898	0.06057	ppb	98
22) Benzo (k) fluoranthene	12.21	252	1083	-0.34909	ppb	97
23) Benzo (a) pyrene	12.74	252	850	-0.08634	ppb	97
25) Benzo (g,h,i) perylene	14.71	276	975	-0.13423	ppb	96

Quantitation Report


Data File : M:\KYLO\DATA\211019\1019K003.D  
Acq On : 19 Oct 21 14:29  
Sample : 0.2 ug/ml 10/13/21  
Misc :

Vial: 3  
Operator: LS  
Inst : KYLO  
Multiplr: 1.00

Quant Time: Oct 19 15:48 2021

Quant Results File: K1019.RES

Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)  
Title : EPA 8270  
Last Update : Tue Nov 09 10:14:45 2021  
Response via : Initial Calibration



Data File : M:\KYLO\DATA\211019\1019K004.D  
 Acq On : 19 Oct 21 14:49  
 Sample : 0.5 ug/ml 10/13/21  
 Misc :

Vial: 4  
 Operator: LS  
 Inst : KYLO  
 Multiplr: 1.00

Quant Time: Oct 19 15:48 2021

Quant Results File: K1019.RES

Quant Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)  
 Title : EPA 8270  
 Last Update : Tue Oct 19 16:47:23 2021  
 Response via : Initial Calibration  
 DataAcq Meth : SIM\_2

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Naphthalene-D8 (IS)	3.92	136	11385	2.50000	ppb	0.00
6) Acenaphthene-D10 (IS)	5.86	164	5536	2.50000	ppb	0.00
10) Phenanthrene-D10 (IS)	7.56	188	8686	2.50000	ppb	0.00
15) Chrysene-D12 (IS)	10.62	240	9708	2.50000	ppb	0.00
20) Perylene-D12 (IS)	12.84	264	8669	2.50000	ppb	0.00
System Monitoring Compounds						
3) 2-Methylnaphthalene-D10 (2)	4.66	152	1507	0.25921	ppb	0.00
Spiked Amount	5.000		Recovery	=	5.180%	
13) Fluoranthene-D10 (FRT)	8.94	212	1646	0.24309	ppb	0.00
Spiked Amount	5.000		Recovery	=	4.860%	
Target Compounds						
						Qvalue
2) Naphthalene	3.94	128	3083	0.52131	ppb	99
4) 2-Methylnaphthalene	4.69	142	1766	0.50952	ppb	99
5) 1-Methylnaphthalene	4.80	142	1806	0.51630	ppb	96
7) Acenaphthylene	5.69	152	5894	0.51427	ppb	100
8) Acenaphthene	5.89	154	1552	0.51126	ppb	100
9) Fluorene	6.49	166	1772	0.50373	ppb	99
11) Phenanthrene	7.59	178	2402	0.50250	ppb	99
12) Anthracene	7.65	178	2259	0.50035	ppb	99
14) Fluoranthene	8.96	202	3711	0.49974	ppb	99
16) Pyrene	9.21	202	3805	0.51191	ppb	98
17) Benz (a) anthracene	10.61	228	2678	0.49216	ppb	99
18) Chrysene	10.65	228	3122	0.51607	ppb	99
19) Indeno (1,2,3-cd) pyrene	14.39	276	2640	0.77101	ppb	# 97
21) Benzo (b) fluoranthene	12.15	252	2255	0.32301	ppb	100
23) Benzo (a) pyrene	12.74	252	2122	0.17741	ppb	99
24) Dibenz (a,h) anthracene	14.43	278	2117	0.29983	ppb	99
25) Benzo (g,h,i) perylene	14.70	276	2445	0.16843	ppb	100

Quantitation Report


Data File : M:\KYLO\DATA\211019\1019K004.D  
Acq On : 19 Oct 21 14:49  
Sample : 0.5 ug/ml 10/13/21  
Misc :

Vial: 4  
Operator: LS  
Inst : KYLO  
Multiplr: 1.00

Quant Time: Oct 19 15:48 2021

Quant Results File: K1019.RES

Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)  
Title : EPA 8270  
Last Update : Tue Nov 09 10:14:45 2021  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data File : M:\KYLO\DATA\211019\1019K005.D  
 Acq On : 19 Oct 21 15:09  
 Sample : 1 ug/ml 10/13/21  
 Misc :

Vial: 5  
 Operator: LS  
 Inst : KYLO  
 Multiplr: 1.00

Quant Time: Oct 19 15:48 2021

Quant Results File: K1019.RES

Quant Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)  
 Title : EPA 8270  
 Last Update : Tue Oct 19 16:47:23 2021  
 Response via : Initial Calibration  
 DataAcq Meth : SIM\_2

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Naphthalene-D8 (IS)	3.92	136	11032	2.50000	ppb	0.00
6) Acenaphthene-D10 (IS)	5.86	164	5365	2.50000	ppb	0.00
10) Phenanthrene-D10 (IS)	7.56	188	8424	2.50000	ppb	0.00
15) Chrysene-D12 (IS)	10.63	240	9455	2.50000	ppb	0.01
20) Perylene-D12 (IS)	12.84	264	8423	2.50000	ppb	0.01
System Monitoring Compounds						
3) 2-Methylnaphthalene-D10 (2)	4.66	152	2880	0.51122	ppb	0.00
Spiked Amount	5.000		Recovery	=	10.220%	
13) Fluoranthene-D10 (FRT)	8.94	212	3208	0.48851	ppb	0.00
Spiked Amount	5.000		Recovery	=	9.780%	
Target Compounds						
						Qvalue
2) Naphthalene	3.94	128	5894	1.02851	ppb	99
4) 2-Methylnaphthalene	4.69	142	3426	1.02008	ppb	99
5) 1-Methylnaphthalene	4.80	142	3513	1.03643	ppb	98
7) Acenaphthylene	5.70	152	11284	1.01594	ppb	99
8) Acenaphthene	5.89	154	2945	1.00106	ppb	97
9) Fluorene	6.49	166	3412	1.00086	ppb	99
11) Phenanthrene	7.59	178	4641	1.00109	ppb	99
12) Anthracene	7.65	178	4379	1.00008	ppb	100
14) Fluoranthene	8.96	202	7234	1.00447	ppb	100
16) Pyrene	9.21	202	7407	1.02317	ppb	99
17) Benz (a) anthracene	10.61	228	5224	0.98576	ppb	99
18) Chrysene	10.65	228	5954	1.01055	ppb	99
19) Indeno (1,2,3-cd) pyrene	14.39	276	5309	1.38990	ppb	# 90
21) Benzo (b) fluoranthene	12.15	252	4568	0.79546	ppb	99
22) Benzo (k) fluoranthene	12.21	252	5497	0.53419	ppb	98
23) Benzo (a) pyrene	12.74	252	4263	0.64650	ppb	99
24) Dibenz (a,h) anthracene	14.44	278	4288	0.78667	ppb	99
25) Benzo (g,h,i) perylene	14.71	276	4733	0.66726	ppb	99

Quantitation Report


Data File : M:\KYLO\DATA\211019\1019K005.D  
Acq On : 19 Oct 21 15:09  
Sample : 1 ug/ml 10/13/21  
Misc :

Vial: 5  
Operator: LS  
Inst : KYLO  
Multiplr: 1.00

Quant Time: Oct 19 15:48 2021

Quant Results File: K1019.RES

Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)  
Title : EPA 8270  
Last Update : Tue Nov 09 10:14:45 2021  
Response via : Initial Calibration



Data File : M:\KYLO\DATA\211019\1019K006.D  
 Acq On : 19 Oct 21 15:29  
 Sample : 5 ug/ml 10/13/21  
 Misc :

Vial: 6  
 Operator: LS  
 Inst : KYLO  
 Multiplr: 1.00

Quant Time: Oct 19 15:48 2021

Quant Results File: K1019.RES

Quant Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)  
 Title : EPA 8270  
 Last Update : Tue Oct 19 16:47:23 2021  
 Response via : Initial Calibration  
 DataAcq Meth : SIM\_2

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Napthalene-D8 (IS)	3.92	136	11022	2.50000	ppb	0.00
6) Acenaphthene-D10 (IS)	5.86	164	5414	2.50000	ppb	0.00
10) Phenanthrene-D10 (IS)	7.56	188	8482	2.50000	ppb	0.00
15) Chrysene-D12 (IS)	10.62	240	10015	2.50000	ppb	0.00
20) Perylene-D12 (IS)	12.83	264	8704	2.50000	ppb	0.00
System Monitoring Compounds						
3) 2-Methylnaphthalene-D10 (2)	4.66	152	14500	2.57619	ppb	0.00
Spiked Amount	5.000		Recovery	=	51.520%	
13) Fluoranthene-D10 (FRT)	8.93	212	17235	2.60659	ppb	0.00
Spiked Amount	5.000		Recovery	=	52.140%	
Target Compounds						
2) Napthalene	3.94	128	28832	5.03578	ppb	100
4) 2-Methylnaphthalene	4.69	142	17384	5.18072	ppb	100
5) 1-Methylnaphthalene	4.80	142	17464	5.15700	ppb	100
7) Acenaphthylene	5.69	152	58890	5.25410	ppb	100
8) Acenaphthene	5.89	154	15136	5.09845	ppb	100
9) Fluorene	6.49	166	17780	5.16829	ppb	100
11) Phenanthrene	7.59	178	23796	5.09785	ppb	100
12) Anthracene	7.64	178	22931	5.20117	ppb	100
14) Fluoranthene	8.95	202	38260	5.27621	ppb	100
16) Pyrene	9.21	202	39012	5.08763	ppb	100
17) Benz (a) anthracene	10.61	228	28070	5.00058	ppb	100
18) Chrysene	10.65	228	31118	4.98620	ppb	100
19) Indeno (1,2,3-cd) pyrene	14.38	276	20323	4.52699	ppb	100
21) Benzo (b) fluoranthene	12.14	252	26309	4.94784	ppb	100
22) Benzo (k) fluoranthene	12.19	252	29066	5.02910	ppb	100
23) Benzo (a) pyrene	12.73	252	25103	4.91484	ppb	100
24) Dibenz (a,h) anthracene	14.42	278	24331	4.98885	ppb	100
25) Benzo (g,h,i) perylene	14.69	276	26049	4.99985	ppb	100



Quantitation Report


Data File : M:\KYLO\DATA\211019\1019K006.D  
Acq On : 19 Oct 21 15:29  
Sample : 5 ug/ml 10/13/21  
Misc :

Vial: 6  
Operator: LS  
Inst : KYLO  
Multiplr: 1.00

Quant Time: Oct 19 15:48 2021

Quant Results File: K1019.RES

Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)  
Title : EPA 8270  
Last Update : Tue Nov 09 10:14:45 2021  
Response via : Initial Calibration



Data File : M:\KYLO\DATA\211019\1019K007.D Vial: 7  
 Acq On : 19 Oct 21 15:49 Operator: LS  
 Sample : 10 ug/ml 10/13/21 Inst : KYLO  
 Misc : Multiplr: 1.00

Quant Time: Oct 19 15:49 2021 Quant Results File: K1019.RES

Quant Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)  
 Title : EPA 8270  
 Last Update : Tue Oct 19 16:47:23 2021  
 Response via : Initial Calibration  
 DataAcq Meth : SIM\_2

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Napthalene-D8 (IS)	3.92	136	11510	2.50000	ppb	0.00
6) Acenaphthene-D10 (IS)	5.86	164	5675	2.50000	ppb	0.00
10) Phenanthrene-D10 (IS)	7.56	188	8972	2.50000	ppb	0.00
15) Chrysene-D12 (IS)	10.62	240	10664	2.50000	ppb	0.00
20) Perylene-D12 (IS)	12.83	264	9232	2.50000	ppb	0.00
System Monitoring Compounds						
3) 2-Methylnaphthalene-D10 (2)	4.66	152	26676	4.53854	ppb	0.00
Spiked Amount	5.000		Recovery	=	90.780%	
13) Fluoranthene-D10 (FRT)	8.93	212	34413	4.92032	ppb	0.00
Spiked Amount	5.000		Recovery	=	98.400%	
Target Compounds						
2) Naphthalene	3.94	128	59354	9.92720	ppb	100
4) 2-Methylnaphthalene	4.69	142	35959	10.26203	ppb	100
5) 1-Methylnaphthalene	4.80	142	35938	10.16232	ppb	100
7) Acenaphthylene	5.69	152	122704	10.44402	ppb	100
8) Acenaphthene	5.89	154	31359	10.07724	ppb	99
9) Fluorene	6.49	166	37236	10.32596	ppb	99
11) Phenanthrene	7.59	178	49310	9.98682	ppb	100
12) Anthracene	7.64	178	48395	10.37738	ppb	100
14) Fluoranthene	8.95	202	79898	10.41651	ppb	100
16) Pyrene	9.21	202	82191	10.06635	ppb	100
17) Benz (a) anthracene	10.61	228	60563	10.13248	ppb	100
18) Chrysene	10.65	228	64649	9.72861	ppb	99
19) Indeno (1,2,3-cd) pyrene	14.38	276	44868	9.18248	ppb	# 99
21) Benzo (b) fluoranthene	12.14	252	55900	10.02449	ppb	99
22) Benzo (k) fluoranthene	12.19	252	63873	11.01716	ppb	99
23) Benzo (a) pyrene	12.73	252	54783	10.38939	ppb	99
24) Dibenz (a,h) anthracene	14.42	278	51533	10.11061	ppb	98
25) Benzo (g,h,i) perylene	14.69	276	56013	10.47964	ppb	98

Quantitation Report


Data File : M:\KYLO\DATA\211019\1019K007.D  
Acq On : 19 Oct 21 15:49  
Sample : 10 ug/ml 10/13/21  
Misc :

Vial: 7  
Operator: LS  
Inst : KYLO  
Multiplr: 1.00

Quant Time: Oct 19 15:49 2021

Quant Results File: K1019.RES

Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)  
Title : EPA 8270  
Last Update : Tue Nov 09 10:14:45 2021  
Response via : Initial Calibration



Data File : M:\KYLO\DATA\211019\1019K008.D  
 Acq On : 19 Oct 21 16:09  
 Sample : 50 ug/ml 10/13/21  
 Misc :

Vial: 8  
 Operator: LS  
 Inst : KYLO  
 Multiplr: 1.00

Quant Time: Oct 19 15:49 2021

Quant Results File: K1019.RES

Quant Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)  
 Title : EPA 8270  
 Last Update : Tue Oct 19 16:47:23 2021  
 Response via : Initial Calibration  
 DataAcq Meth : SIM\_2

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Napthalene-D8 (IS)	3.92	136	11542	2.50000	ppb	0.00
6) Acenaphthene-D10 (IS)	5.86	164	5767	2.50000	ppb	0.00
10) Phenanthrene-D10 (IS)	7.56	188	8902	2.50000	ppb	0.00
15) Chrysene-D12 (IS)	10.62	240	10648	2.50000	ppb	0.00
20) Perylene-D12 (IS)	12.83	264	9592	2.50000	ppb	0.00
System Monitoring Compounds						
3) 2-Methylnaphthalene-D10 (2)	4.66	152	140995	23.92178	ppb	0.00
Spiked Amount	5.000		Recovery	=	478.440%	
13) Fluoranthene-D10 (FRT)	8.93	212	173855	25.05302	ppb	0.00
Spiked Amount	5.000		Recovery	=	501.060%	
Target Compounds						
						Qvalue
2) Naphthalene	3.94	128	270597	45.13299	ppb	100
4) 2-Methylnaphthalene	4.69	142	165624	47.13496	ppb	99
5) 1-Methylnaphthalene	4.80	142	164402	46.35966	ppb	99
7) Acenaphthylene	5.70	152	560845	46.97510	ppb	100
8) Acenaphthene	5.89	154	145964	46.15736	ppb	99
9) Fluorene	6.49	166	175391	47.86199	ppb	100
11) Phenanthrene	7.59	178	233010	47.56290	ppb	100
12) Anthracene	7.64	178	228704	49.42683	ppb	100
14) Fluoranthene	8.96	202	371445	48.80706	ppb	99
16) Pyrene	9.21	202	379423	46.53971	ppb	98
17) Benz (a) anthracene	10.61	228	291856	48.90228	ppb	100
18) Chrysene	10.65	228	300277	45.25466	ppb	99
19) Indeno (1,2,3-cd) pyrene	14.38	276	248943	50.15933	ppb	94
21) Benzo (b) fluoranthene	12.15	252	294828	51.34534	ppb	99
22) Benzo (k) fluoranthene	12.20	252	302763	52.24864	ppb	100
23) Benzo (a) pyrene	12.73	252	278840	51.91758	ppb	100
24) Dibenz (a,h) anthracene	14.42	278	268409	51.28254	ppb	97
25) Benzo (g,h,i) perylene	14.70	276	280479	51.78283	ppb	99

Quantitation Report


Data File : M:\KYLO\DATA\211019\1019K008.D  
 Acq On : 19 Oct 21 16:09  
 Sample : 50 ug/ml 10/13/21  
 Misc :

Vial: 8  
 Operator: LS  
 Inst : KYLO  
 Multiplr: 1.00

Quant Time: Oct 19 15:49 2021

Quant Results File: K1019.RES

Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)  
 Title : EPA 8270  
 Last Update : Tue Nov 09 10:14:45 2021  
 Response via : Initial Calibration



Data File : M:\KYLO\DATA\211019\1019K009.D  
 Acq On : 19 Oct 21 16:29  
 Sample : 100 ug/ml 10/13/21  
 Misc :

Vial: 9  
 Operator: LS  
 Inst : KYLO  
 Multiplr: 1.00

Quant Time: Oct 19 15:49 2021

Quant Results File: K1019.RES

Quant Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)  
 Title : EPA 8270  
 Last Update : Tue Oct 19 16:47:23 2021  
 Response via : Initial Calibration  
 DataAcq Meth : SIM\_2

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Napthalene-D8 (IS)	3.92	136	11679	2.50000	ppb	0.00
6) Acenaphthene-D10 (IS)	5.86	164	5877	2.50000	ppb	0.00
10) Phenanthrene-D10 (IS)	7.56	188	9024	2.50000	ppb	0.00
15) Chrysene-D12 (IS)	10.63	240	10469	2.50000	ppb	0.01
20) Perylene-D12 (IS)	12.83	264	9899	2.50000	ppb	0.00
System Monitoring Compounds						
3) 2-Methylnaphthalene-D10 (2)	4.66	152	278374	46.67602	ppb	0.00
Spiked Amount	5.000		Recovery	=	933.520%	
13) Fluoranthene-D10 (FRT)	8.94	212	341108	48.49012	ppb	0.00
Spiked Amount	5.000		Recovery	=	969.800%	
Target Compounds						
2) Napthalene	3.94	128	514066	84.73550	ppb	100
4) 2-Methylnaphthalene	4.70	142	318816	89.66757	ppb	99
5) 1-Methylnaphthalene	4.80	142	317528	88.48927	ppb	98
7) Acenaphthylene	5.70	152	1047512	86.09505	ppb	98
8) Acenaphthene	5.90	154	283708	88.03615	ppb	94
9) Fluorene	6.49	166	342219	91.63932	ppb	99
11) Phenanthrene	7.59	178	452383	91.09374	ppb	99
12) Anthracene	7.65	178	447639	95.43451	ppb	100
14) Fluoranthene	8.96	202	701599	90.94222	ppb	97
16) Pyrene	9.22	202	720167	89.84545	ppb	99
17) Benz (a) anthracene	10.62	228	562838	95.91946	ppb	99
18) Chrysene	10.66	228	575910	88.27926	ppb	98
19) Indeno (1,2,3-cd) pyrene	14.39	276	488982	100.01982	ppb	89
21) Benzo (b) fluoranthene	12.16	252	587997	99.33083	ppb	100
22) Benzo (k) fluoranthene	12.16	252	587786	98.78137	ppb	99
23) Benzo (a) pyrene	12.74	252	547488	99.01252	ppb	98
24) Dibenz (a,h) anthracene	14.43	278	535891	99.35185	ppb	94
25) Benzo (g,h,i) perylene	14.71	276	552068	99.06661	ppb	98

Quantitation Report


Data File : M:\KYLO\DATA\211019\1019K009.D  
Acq On : 19 Oct 21 16:29  
Sample : 100 ug/ml 10/13/21  
Misc :

Vial: 9  
Operator: LS  
Inst : KYLO  
Multiplr: 1.00

Quant Time: Oct 19 15:49 2021

Quant Results File: K1019.RES

Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)  
Title : EPA 8270  
Last Update : Tue Nov 09 10:14:45 2021  
Response via : Initial Calibration



PAH by GCMS SIM  
EPA 8270 SIM

Form 7

Second Source Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: \_\_\_\_\_

SDG No: \_\_\_\_\_  
Date Analyzed: 10/19/2021  
Instrument: KYLO  
Initial Cal. Date: 10/19/2021  
Data File: 1019K010.D

		Compound	MEAN	CCRF	%D	%Drift
1	TM	Naphthalene	1.299	1.295	0.25	TM
2	TM	2-Methylnaphthalene	0.7611	0.7635	0.32	TM
3	TM	1-Methylnaphthalene	0.7681	0.7563	1.5	TM
4	TM	Acenaphthylene	5.176	5.272	1.9	TM
5	*TM	Acenaphthene	1.371	1.393	1.6	*TM
6	TM	Fluorene	1.589	1.616	1.7	TM
7	TM	Phenanthrene	1.376	1.380	0.31	TM
8	TM	Anthracene	1.299	1.415	8.9	TM
9	*TM	Fluoranthene	2.137	2.167	1.4	*TM
10	TM	Pyrene	1.914	1.918	0.21	TM
11	TM	Benz (a) anthracene	1.401	1.374	1.9	TM
12	TM	Chrysene	1.558	1.488	4.5	TM
13	TML	Indeno (1,2,3-cd) pyrene	1.272	0.9799	23	TML 12
14	TM	Benzo (b) fluoranthene	1.408	1.510	7.3	TM
15	TM	Benzo (k) fluoranthene	1.610	1.698	5.5	TM
16	*TM	Benzo (a) pyrene	1.341	1.484	11	*TM
17	TM	Dibenz (a,h) anthracene	1.326	1.382	4.2	TM
18	TM	Benzo (g,h,i) perylene	1.443	1.486	3.0	TM
19						
20						
21						
22						
23						
24						
25						
26						
27						
28						
29						
30						
31						
32						
33						
34						
35						
36						
37						
38						

Average

4.4

PAH by GCMS SIM  
EPA 8270 SIM



Data File : M:\KYLO\DATA\211019\1019K010.D  
 Acq On : 19 Oct 21 16:49  
 Sample : SS ug/ml 10/13/21  
 Misc :

Vial: 10  
 Operator: LS  
 Inst : KYLO  
 Multiplr: 1.00

Quant Time: Oct 19 16:06 2021

Quant Results File: K1019.RES

Quant Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)  
 Title : EPA 8270  
 Last Update : Tue Oct 19 16:51:19 2021  
 Response via : Initial Calibration  
 DataAcq Meth : SIM\_2

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Napthalene-D8(IS)	3.92	136	11540	2.50000	ppb	0.00
6) Acenaphthene-D10(IS)	5.86	164	5722	2.50000	ppb	0.00
10) Phenanthrene-D10(IS)	7.56	188	8843	2.50000	ppb	0.00
15) Chrysene-D12(IS)	10.62	240	10394	2.50000	ppb	0.00
20) Perylene-D12(IS)	12.83	264	8800	2.50000	ppb	0.00

System Monitoring Compounds

3) 2-Methylnaphthalene-D10 (2)	4.66	152	1	0.00017	ppb	0.00
Spiked Amount	5.000		Recovery	=	0.000%	
13) Fluoranthene-D10 (FRT)	8.93	212	9	0.00131	ppb	0.00
Spiked Amount	5.000		Recovery	=	0.020%	

Target Compounds

	R.T.	QIon	Response	Conc	Units	Qvalue
2) Naphthalene	3.94	128	29897	4.98740	ppb	100
4) 2-Methylnaphthalene	4.69	142	17622	5.01592	ppb	100
5) 1-Methylnaphthalene	4.80	142	17455	4.92298	ppb	100
7) Acenaphthylene	5.69	152	60338	5.09352	ppb	100
8) Acenaphthene	5.89	154	15936	5.07898	ppb	100
9) Fluorene	6.49	166	18488	5.08482	ppb	100
11) Phenanthrene	7.59	178	24407	5.01529	ppb	100
12) Anthracene	7.64	178	25019	5.44311	ppb	100
14) Fluoranthene	8.95	202	38328	5.06982	ppb	99
16) Pyrene	9.21	202	39873	5.01031	ppb	100
17) Benz (a) anthracene	10.61	228	28567	4.90355	ppb	99
18) Chrysene	10.65	228	30939	4.77675	ppb	100
19) Indeno (1,2,3-cd) pyrene	14.38	276	20371	4.37871	ppb	99
21) Benzo (b) fluoranthene	12.14	252	26577	5.36265	ppb	100
22) Benzo (k) fluoranthene	12.19	252	29888	5.27373	ppb	100
23) Benzo (a) pyrene	12.73	252	26127	5.53492	ppb	100
24) Dibenz (a,h) anthracene	14.42	278	24324	5.21145	ppb	99
25) Benzo (g,h,i) perylene	14.69	276	26159	5.14999	ppb	100

Quantitation Report


Data File : M:\KYLO\DATA\211019\1019K010.D  
Acq On : 19 Oct 21 16:49  
Sample : SS ug/ml 10/13/21  
Misc :

Vial: 10  
Operator: LS  
Inst : KYLO  
Multiplr: 1.00

Quant Time: Oct 19 16:06 2021

Quant Results File: K1019.RES

Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)  
Title : EPA 8270  
Last Update : Tue Nov 09 10:14:45 2021  
Response via : Initial Calibration



PAH by GCMS SIM  
EPA 8270 SIM

Form 7

Continuing Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: \_\_\_\_\_

SDG No: \_\_\_\_\_  
Date Analyzed: 11/18/2021  
Instrument: KYLO  
Initial Cal. Date: 10/19/2021  
Data File: 1019K437.D

		Compound	MEAN	CCRF	%D	%Drift
1	I	Napthalene-D8(IS)	ISTD			I
2	TM	Napthalene	1.299	1.339	3.1	TM
3	S	2-Methylnapthalene-D10 (2MN)	1.277	1.295	1.5	S
4	TM	2-Methylnapthalene	0.7611	0.8111	6.6	TM
5	TM	1-Methylnapthalene	0.7681	0.8098	5.4	TM
6	I	Acenaphthene-D10(IS)	ISTD			I
7	TM	Acenaphthylene	5.176	5.616	8.5	TM
8	*TM	Acenaphthene	1.371	1.443	5.3	*TM
9	TM	Fluorene	1.589	1.671	5.2	TM
10	I	Phenanthrene-D10(IS)	ISTD			I
11	TM	Phenanthrene	1.376	1.473	7.0	TM
12	TM	Anthracene	1.299	1.433	10	TM
13	S	Fluoranthene-D10 (FRT)	1.949	2.044	4.9	S
14	*TM	Fluoranthene	2.137	2.376	11	*TM
15	I	Chrysene-D12(IS)	ISTD			I
16	TM	Pyrene	1.914	2.011	5.1	TM
17	TM	Benz (a) anthracene	1.401	1.549	11	TM
18	TM	Chrysene	1.558	1.561	0.18	TM
19	TML	Indeno (1,2,3-cd) pyrene	1.272	1.175	7.7	TML 4.2
20	I	Perylene-D12(IS)	ISTD			I
21	TM	Benzo (b) fluoranthene	1.408	1.588	13	TM
22	TM	Benzo (k) fluoranthene	1.610	1.654	2.7	TM
23	*TM	Benzo (a) pyrene	1.341	1.477	10	*TM
24	TM	Dibenz (a,h) anthracene	1.326	1.375	3.7	TM
25	TM	Benzo (g,h,i) perylene	1.443	1.517	5.1	TM
26						
27						
28						
29						
30						
31						
32						
33						
34						
35						
36						
37						
38						
39						
40						

Average

6.3

Quantitation Report (Not Reviewed)

Data File : M:\KYLO\DATA\211019\1019K437.D Vial: 137  
 Acq On : 18 Nov 21 9:01 Operator: LS  
 Sample : 5 ug/ml 10/19/21 (1) Inst : KYLO  
 Misc : Multiplr: 1.00

Quant Time: Nov 18 9:17 2021 Quant Results File: K1019.RES

Quant Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)  
 Title : EPA 8270  
 Last Update : Tue Nov 09 10:14:45 2021  
 Response via : Initial Calibration  
 DataAcq Meth : SIM\_2

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Naphthalene-D8 (IS)	3.86	136	12784	2.50000	ppb	-0.03
6) Acenaphthene-D10 (IS)	5.80	164	6153	2.50000	ppb	-0.06
10) Phenanthrene-D10 (IS)	7.49	188	9197	2.50000	ppb	-0.06
15) Chrysene-D12 (IS)	10.54	240	11234	2.50000	ppb	-0.07
20) Perylene-D12 (IS)	12.71	264	10043	2.50000	ppb	-0.13
<b>System Monitoring Compounds</b>						
3) 2-Methylnaphthalene-D10 (2)	4.59	152	16561	2.53683	ppb	-0.06
Spiked Amount	5.000		Recovery	=	50.740%	
13) Fluoranthene-D10 (FRT)	8.86	212	18795	2.62154	ppb	-0.07
Spiked Amount	5.000		Recovery	=	52.440%	
<b>Target Compounds</b>						
						Qvalue
2) Naphthalene	3.88	128	34223	5.15351	ppb	100
4) 2-Methylnaphthalene	4.63	142	20738	5.32845	ppb	100
5) 1-Methylnaphthalene	4.74	142	20704	5.27111	ppb	100
7) Acenaphthylene	5.63	152	69115	5.42576	ppb	99
8) Acenaphthene	5.83	154	17758	5.26323	ppb	99
9) Fluorene	6.42	166	20561	5.25885	ppb	98
11) Phenanthrene	7.52	178	27090	5.35235	ppb	100
12) Anthracene	7.58	178	26361	5.51432	ppb	99
14) Fluoranthene	8.89	202	43705	5.55854	ppb	97
16) Pyrene	9.14	202	45181	5.25278	ppb	99
17) Benz (a) anthracene	10.53	228	34792	5.52552	ppb	99
18) Chrysene	10.57	228	35064	5.00883	ppb	99
19) Indeno (1,2,3-cd) pyrene	14.28	276	26397	5.21198	ppb	# 97
21) Benzo (b) fluoranthene	12.03	252	31894	5.63899	ppb	98
22) Benzo (k) fluoranthene	12.08	252	33227	5.13726	ppb	99
23) Benzo (a) pyrene	12.60	252	29670	5.50755	ppb	97
24) Dibenz (a,h) anthracene	14.32	278	27610	5.18334	ppb	99
25) Benzo (g,h,i) perylene	14.59	276	30463	5.25505	ppb	99

Quantitation Report


Data File : M:\KYLO\DATA\211019\1019K437.D  
Acq On : 18 Nov 21 9:01  
Sample : 5 ug/ml 10/19/21 (1)  
Misc :

Vial: 137  
Operator: LS  
Inst : KYLO  
Multiplr: 1.00

Quant Time: Nov 18 9:17 2021

Quant Results File: K1019.RES

Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)  
Title : EPA 8270  
Last Update : Tue Nov 09 10:14:45 2021  
Response via : Initial Calibration



PAH by GCMS SIM  
EPA 8270 SIM

Form 7

Ending Continuing Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: \_\_\_\_\_

SDG No: \_\_\_\_\_  
Date Analyzed: 11/18/2021  
Instrument: KYLO  
Initial Cal. Date: 10/19/2021  
Data File: 1019K472.D

		Compound	MEAN	CCRF	%D	%Drift
1	I	Naphthalene-D8(IS)	ISTD			I
2	TM	Naphthalene	1.299	1.303	0.35	TM
3	S	2-Methylnaphthalene-D10 (2MN)	1.277	1.285	0.68	S
4	TM	2-Methylnaphthalene	0.7611	0.7941	4.3	TM
5	TM	1-Methylnaphthalene	0.7681	0.7936	3.3	TM
6	I	Acenaphthene-D10(IS)	ISTD			I
7	TM	Acenaphthylene	5.176	5.586	7.9	TM
8	*TM	Acenaphthene	1.371	1.403	2.3	*TM
9	TM	Fluorene	1.589	1.670	5.1	TM
10	I	Phenanthrene-D10(IS)	ISTD			I
11	TM	Phenanthrene	1.376	1.437	4.5	TM
12	TM	Anthracene	1.299	1.373	5.7	TM
13	S	Fluoranthene-D10 (FRT)	1.949	2.130	9.3	S
14	*TM	Fluoranthene	2.137	2.378	11	*TM
15	I	Chrysene-D12(IS)	ISTD			I
16	TM	Pyrene	1.914	1.967	2.8	TM
17	TM	Benz (a) anthracene	1.401	1.467	4.7	TM
18	TM	Chrysene	1.558	1.535	1.5	TM
19	TML	Indeno (1,2,3-cd) pyrene	1.272	1.101	13	TML 2.1
20	I	Perylene-D12(IS)	ISTD			I
21	TM	Benzo (b) fluoranthene	1.408	1.525	8.3	TM
22	TM	Benzo (k) fluoranthene	1.610	1.619	0.56	TM
23	*TM	Benzo (a) pyrene	1.341	1.436	7.1	*TM
24	TM	Dibenz (a,h) anthracene	1.326	1.289	2.8	TM
25	TM	Benzo (g,h,i) perylene	1.443	1.432	0.79	TM
26						
27						
28						
29						
30						
31						
32						
33						
34						
35						
36						
37						
38						
39						
40						

Average

4.8

Data File : M:\KYLO\DATA\211019\1019K472.D  
 Acq On : 18 Nov 21 20:38  
 Sample : 5 ug/ml 10/13/21 (2)  
 Misc :

Vial: 22  
 Operator: LS  
 Inst : KYLO  
 Multiplr: 1.00

Quant Time: Nov 19 7:35 2021

Quant Results File: K1019.RES

Quant Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)  
 Title : EPA 8270  
 Last Update : Thu Nov 18 11:41:54 2021  
 Response via : Initial Calibration  
 DataAcq Meth : SIM\_2

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Naphthalene-D8 (IS)	3.86	136	14852	2.50000	ppb	0.00
6) Acenaphthene-D10 (IS)	5.79	164	7503	2.50000	ppb	-0.07
10) Phenanthrene-D10 (IS)	7.49	188	11571	2.50000	ppb	-0.07
15) Chrysene-D12 (IS)	10.54	240	14376	2.50000	ppb	-0.07
20) Perylene-D12 (IS)	12.71	264	13027	2.50000	ppb	-0.12
System Monitoring Compounds						
3) 2-Methylnaphthalene-D10 (2)	4.59	152	19089	2.51692	ppb	0.00
Spiked Amount	5.000		Recovery	=	50.340%	
13) Fluoranthene-D10 (FRT)	8.86	212	24641	2.73179	ppb	-0.07
Spiked Amount	5.000		Recovery	=	54.640%	
Target Compounds						
2) Naphthalene	3.89	128	38709	5.01741	ppb	99
4) 2-Methylnaphthalene	4.63	142	23588	5.21684	ppb #	66
5) 1-Methylnaphthalene	4.74	142	23574	5.16610	ppb	86
7) Acenaphthylene	5.63	152	83822	5.39632	ppb	99
8) Acenaphthene	5.83	154	21046	5.11540	ppb	99
9) Fluorene	6.42	166	25063	5.25692	ppb	99
11) Phenanthrene	7.52	178	33256	5.22252	ppb	100
12) Anthracene	7.57	178	31773	5.28280	ppb	100
14) Fluoranthene	8.89	202	55021	5.56203	ppb	100
16) Pyrene	9.14	202	56551	5.13772	ppb	98
17) Benz (a) anthracene	10.53	228	42170	5.23352	ppb	99
18) Chrysene	10.57	228	44132	4.92634	ppb	98
19) Indeno (1,2,3-cd) pyrene	14.28	276	31655	4.89606	ppb	100
21) Benzo (b) fluoranthene	12.02	252	39729	5.41526	ppb	99
22) Benzo (k) fluoranthene	12.07	252	42182	5.02790	ppb	99
23) Benzo (a) pyrene	12.60	252	37420	5.35505	ppb	98
24) Dibenz (a,h) anthracene	14.32	278	33581	4.86022	ppb	98
25) Benzo (g,h,i) perylene	14.58	276	37301	4.96071	ppb	97

Quantitation Report


Data File : M:\KYLO\DATA\211019\1019K472.D  
Acq On : 18 Nov 21 20:38  
Sample : 5 ug/ml 10/13/21 (2)  
Misc :

Vial: 22  
Operator: LS  
Inst : KYLO  
Multiplr: 1.00

Quant Time: Nov 19 7:35 2021

Quant Results File: K1019.RES

Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)  
Title : EPA 8270  
Last Update : Thu Nov 18 11:41:54 2021  
Response via : Initial Calibration

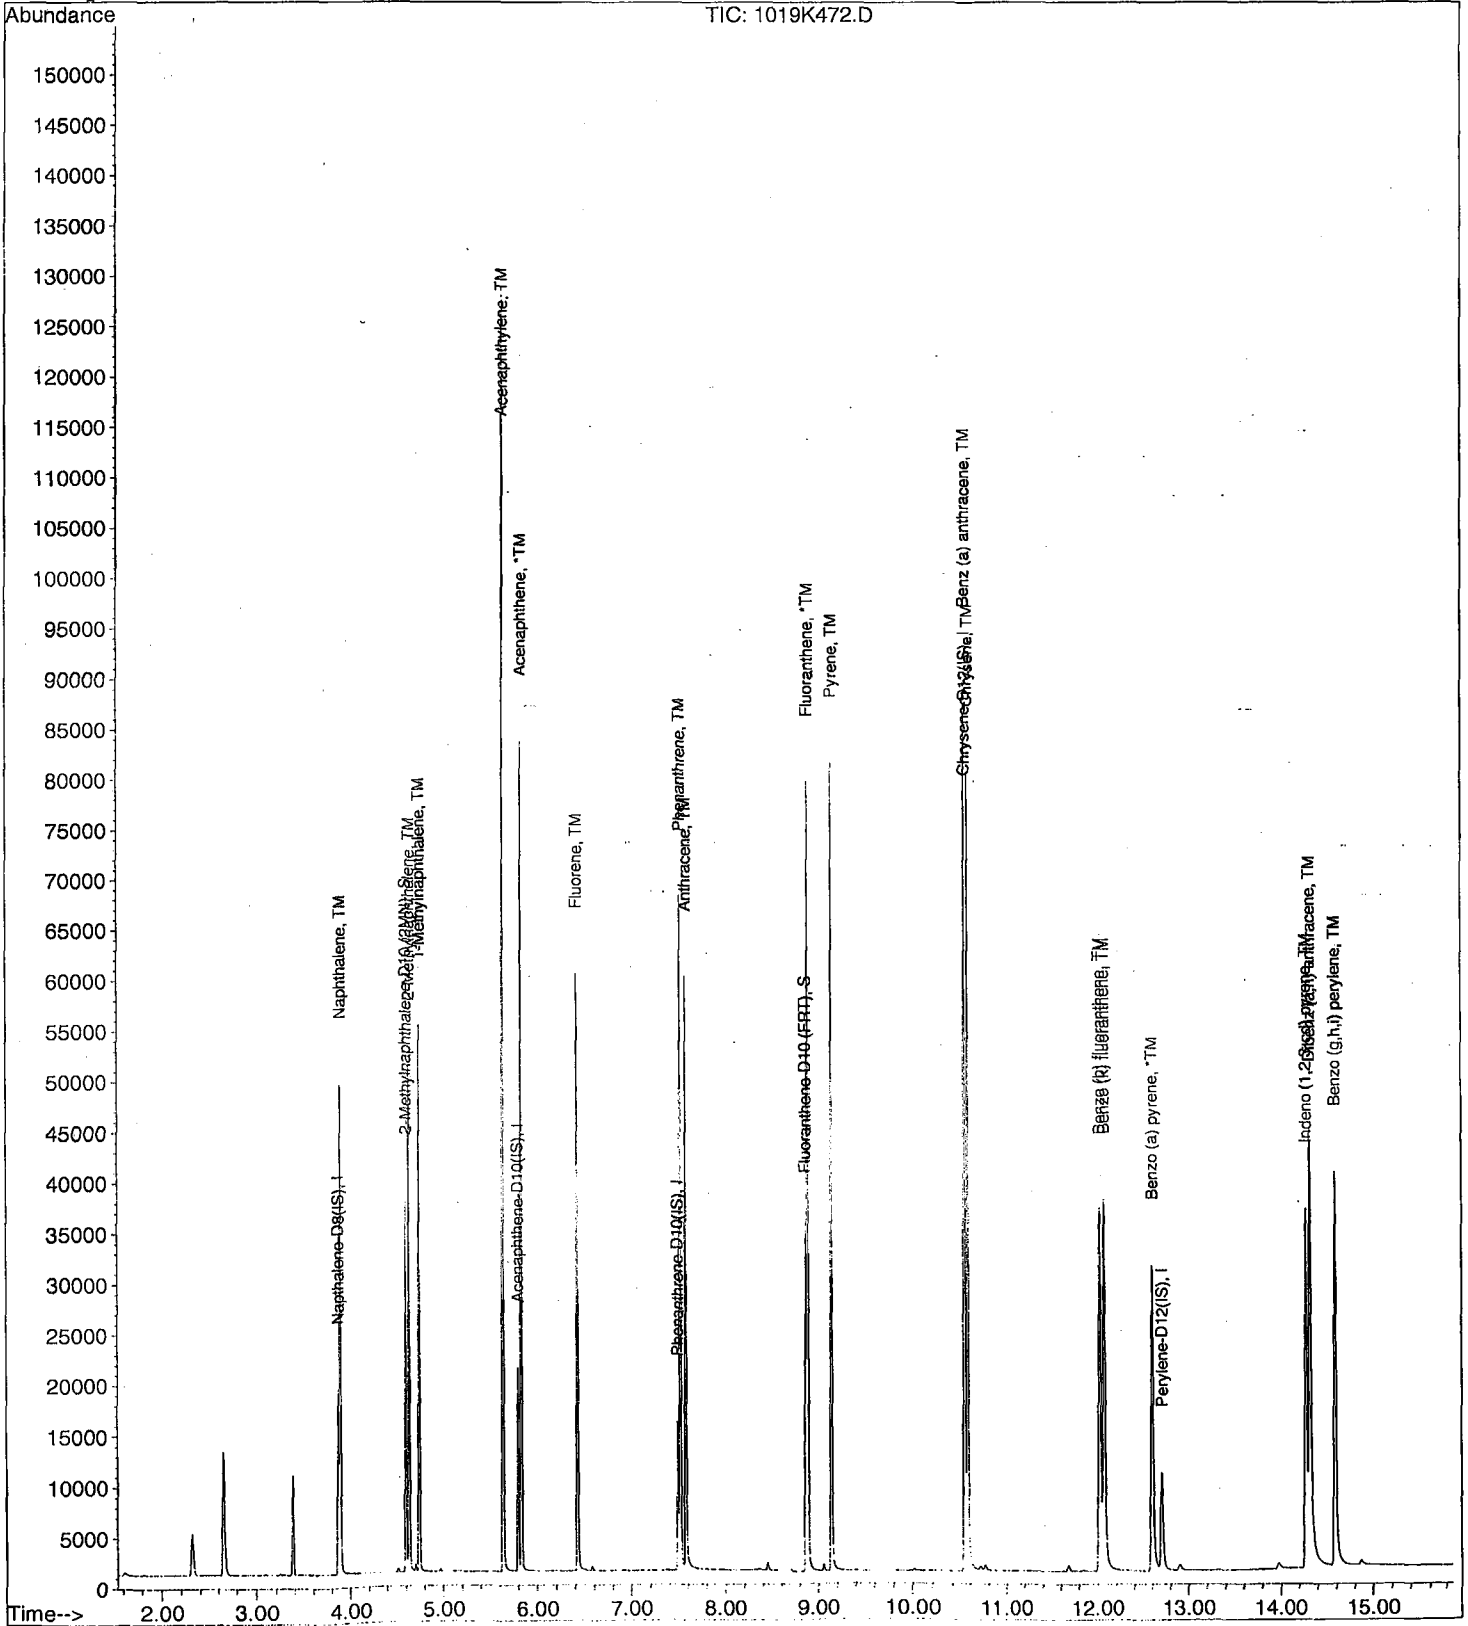



**ORGANICS**  
**Raw Data**

Data File : M:\KYLO\DATA\211019\1019K448.D Vial: 148  
 Acq On : 18 Nov 21 12:40 Operator: LS  
 Sample : BA46115W07 1/1000 Inst : KYLO  
 Misc : Multiplr: 1.00

Quant Time: Nov 18 14:37 2021 Quant Results File: K1019.RES

Quant Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)  
 Title : EPA 8270  
 Last Update : Thu Nov 18 11:41:54 2021  
 Response via : Initial Calibration  
 DataAcq Meth : SIM\_2

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Napthalene-D8 (IS)	3.86	136	14338	2.50000	ppb	0.00
6) Acenaphthene-D10 (IS)	5.79	164	7099	2.50000	ppb	-0.07
10) Phenanthrene-D10 (IS)	7.49	188	10844	2.50000	ppb	-0.06
15) Chrysene-D12 (IS)	10.54	240	13002	2.50000	ppb	-0.07
20) Perylene-D12 (IS)	12.71	264	11849	2.50000	ppb	-0.13
System Monitoring Compounds						
3) 2-Methylnaphthalene-D10 (2)	4.60	152	31234	4.26589	ppb	0.00
Spiked Amount	5.000		Recovery	=	85.320%	
13) Fluoranthene-D10 (FRT)	8.86	212	41596	4.92065	ppb	-0.07
Spiked Amount	5.000		Recovery	=	98.420%	

Target Compounds Qvalue

Quantitation Report


Data File : M:\KYLO\DATA\211019\1019K448.D  
Acq On : 18 Nov 21 12:40  
Sample : BA46115W07 1/1000  
Misc :

Vial: 148  
Operator: LS  
Inst : KYLO  
Multiplr: 1.00

Quant Time: Nov 18 14:37 2021

Quant Results File: K1019.RES

Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)  
Title : EPA 8270  
Last Update : Tue Nov 30 08:16:15 2021  
Response via : Initial Calibration



Data File : M:\KYLO\DATA\211019\1019K449.D Vial: 149  
 Acq On : 18 Nov 21 13:00 Operator: LS  
 Sample : BA46116W05 1/1000 Inst : KYLO  
 Misc : Multiplr: 1.00

Quant Time: Nov 18 14:37 2021 Quant Results File: K1019.RES

Quant Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)  
 Title : EPA 8270  
 Last Update : Thu Nov 18 11:41:54 2021  
 Response via : Initial Calibration  
 DataAcq Meth : SIM\_2

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Napthalene-D8 (IS)	3.86	136	14604	2.50000	ppb	0.00
6) Acenaphthene-D10 (IS)	5.79	164	7118	2.50000	ppb	-0.07
10) Phenanthrene-D10 (IS)	7.49	188	11034	2.50000	ppb	-0.06
15) Chrysene-D12 (IS)	10.54	240	13219	2.50000	ppb	-0.07
20) Perylene-D12 (IS)	12.71	264	12131	2.50000	ppb	-0.13
<b>System Monitoring Compounds</b>						
3) 2-Methylnaphthalene-D10 (2)	4.59	152	35035	4.69787	ppb	0.00
Spiked Amount	5.000		Recovery	=	93.960%	
13) Fluoranthene-D10 (FRT)	8.86	212	43218	5.02449	ppb	-0.07
Spiked Amount	5.000		Recovery	=	100.480%	

Target Compounds Qvalue

Quantitation Report


Data File : M:\KYLO\DATA\211019\1019K449.D  
Acq On : 18 Nov 21 13:00  
Sample : BA46116W05 1/1000  
Misc :

Vial: 149  
Operator: LS  
Inst : KYLO  
Multiplr: 1.00

Quant Time: Nov 18 14:37 2021

Quant Results File: K1019.RES

Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)  
Title : EPA 8270  
Last Update : Tue Nov 30 08:16:15 2021  
Response via : Initial Calibration



Data File : M:\KYLO\DATA\211019\1019K438.D Vial: 138  
 Acq On : 18 Nov 21 9:21 Operator: LS  
 Sample : 211115A BLK 1/1000 Inst : KYLO  
 Misc : Multiplr: 1.00

Quant Time: Nov 18 9:40 2021 Quant Results File: K1019.RES

Quant Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)  
 Title : EPA 8270  
 Last Update : Thu Nov 18 09:39:15 2021  
 Response via : Initial Calibration  
 DataAcq Meth : SIM\_2

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Napthalene-D8 (IS)	3.86	136	12866	2.50000	ppb	0.00
6) Acenaphthene-D10 (IS)	5.79	164	6185	2.50000	ppb	-0.07
10) Phenanthrene-D10 (IS)	7.49	188	9328	2.50000	ppb	-0.06
15) Chrysene-D12 (IS)	10.55	240	11283	2.50000	ppb	-0.07
20) Perylene-D12 (IS)	12.71	264	10568	2.50000	ppb	-0.12

System Monitoring Compounds						
3) 2-Methylnaphthalene-D10 (2)	4.59	152	28143	4.28349	ppb	-0.06
Spiked Amount	5.000		Recovery	=	85.660%	
13) Fluoranthene-D10 (FRT)	8.87	212	36877	5.07140	ppb	-0.07
Spiked Amount	5.000		Recovery	=	101.420%	

Target Compounds Qvalue

Quantitation Report


Data File : M:\KYLO\DATA\211019\1019K438.D  
Acq On : 18 Nov 21 9:21  
Sample : 211115A BLK 1/1000  
Misc :

Vial: 138  
Operator: LS  
Inst : KYLO  
Multiplr: 1.00

Quant Time: Nov 18 9:40 2021

Quant Results File: K1019.RES

Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)  
Title : EPA 8270  
Last Update : Tue Nov 30 08:16:15 2021  
Response via : Initial Calibration



Data File : M:\KYLO\DATA\211019\1019K439.D  
 Acq On : 18 Nov 21 9:40  
 Sample : 211115A LCS-1 1/1000  
 Misc :

Vial: 139  
 Operator: LS  
 Inst : KYLO  
 Multiplr: 1.00

Quant Time: Nov 18 10:00 2021

Quant Results File: K1019.RES

Quant Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)  
 Title : EPA 8270  
 Last Update : Thu Nov 18 10:00:46 2021  
 Response via : Initial Calibration  
 DataAcq Meth : SIM\_2

Internal Standards	R.T.	QI on	Response	Conc	Units	Dev (Min)
1) Napthalene-D8 (IS)	3.86	136	12352	2.50000	ppb	0.00
6) Acenaphthene-D10 (IS)	5.79	164	6114	2.50000	ppb	-0.07
10) Phenanthrene-D10 (IS)	7.49	188	9269	2.50000	ppb	-0.06
15) Chrysene-D12 (IS)	10.54	240	11195	2.50000	ppb	-0.07
20) Perylene-D12 (IS)	12.71	264	10472	2.50000	ppb	-0.13

System Monitoring Compounds	R.T.	QI on	Response	Conc	Units	Dev (Min)
3) 2-Methylnaphthalene-D10 (2)	4.59	152	28469	4.51342	ppb	-0.06
Spiked Amount	5.000		Recovery	=	90.260%	
13) Fluoranthene-D10 (FRT)	8.86	212	36454	5.04513	ppb	-0.07
Spiked Amount	5.000		Recovery	=	100.900%	

Target Compounds	R.T.	QI on	Response	Conc	Units	Qvalue
2) Naphthalene	3.88	128	25551	3.98220	ppb	100
4) 2-Methylnaphthalene	4.63	142	15297	4.06790	ppb	100
5) 1-Methylnaphthalene	4.74	142	15329	4.03916	ppb	100
7) Acenaphthylene	5.63	152	52725	4.16549	ppb	99
8) Acenaphthene	5.83	154	13708	4.08878	ppb	98
9) Fluorene	6.42	166	16036	4.12766	ppb	98
11) Phenanthrene	7.52	178	21413	4.19784	ppb	100
12) Anthracene	7.57	178	20044	4.16033	ppb	100
14) Fluoranthene	8.89	202	34932	4.40825	ppb	100
16) Pyrene	9.14	202	35938	4.19274	ppb	100
17) Benz (a) anthracene	10.53	228	27124	4.32273	ppb	99
18) Chrysene	10.57	228	28289	4.05511	ppb	99
19) Indeno (1,2,3-cd) pyrene	14.28	276	20381	4.08091	ppb	95
21) Benzo (b) fluoranthene	12.03	252	25973	4.40401	ppb	99
22) Benzo (k) fluoranthene	12.08	252	27675	4.10357	ppb	99
23) Benzo (a) pyrene	12.60	252	23366	4.15967	ppb	99
24) Dibenz (a,h) anthracene	14.32	278	22654	4.07870	ppb	96
25) Benzo (g,h,i) perylene	14.59	276	24558	4.06286	ppb	99

(#) = qualifier out of range (m) = manual integration



Quantitation Report


Data File : M:\KYLO\DATA\211019\1019K439.D  
Acq On : 18 Nov 21 9:40  
Sample : 211115A LCS-1 1/1000  
Misc :

Vial: 139  
Operator: LS  
Inst : KYLO  
Multiplr: 1.00

Quant Time: Nov 18 10:00 2021

Quant Results File: K1019.RES

Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)  
Title : EPA 8270  
Last Update : Tue Nov 30 08:16:15 2021  
Response via : Initial Calibration



Data File : M:\KYLO\DATA\211019\1019K440.D Vial: 140  
 Acq On : 18 Nov 21 10:00 Operator: LS  
 Sample : 211115A LCSD-1 1/1000 Inst : KYLO  
 Misc : Multiplr: 1.00

Quant Time: Nov 18 10:20 2021 Quant Results File: K1019.RES

Quant Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)  
 Title : EPA 8270  
 Last Update : Thu Nov 18 10:00:46 2021  
 Response via : Initial Calibration  
 DataAcq Meth : SIM\_2

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Napthalene-D8 (IS)	3.86	136	12851	2.50000	ppb	0.00
6) Acenaphthene-D10 (IS)	5.79	164	6340	2.50000	ppb	-0.07
10) Phenanthrene-D10 (IS)	7.49	188	9491	2.50000	ppb	-0.06
15) Chrysene-D12 (IS)	10.54	240	11677	2.50000	ppb	-0.07
20) Perylene-D12 (IS)	12.71	264	10742	2.50000	ppb	-0.12
<b>System Monitoring Compounds</b>						
3) 2-Methylnaphthalene-D10 (2)	4.59	152	28986	4.41695	ppb	-0.06
Spiked Amount	5.000		Recovery	=	88.340%	
13) Fluoranthene-D10 (FRT)	8.86	212	35741	4.83076	ppb	-0.07
Spiked Amount	5.000		Recovery	=	96.620%	
<b>Target Compounds</b>						
						Qvalue
2) Naphthalene	3.89	128	24264	3.63478	ppb	99
4) 2-Methylnaphthalene	4.63	142	14516	3.71032	ppb	99
5) 1-Methylnaphthalene	4.74	142	14431	3.65489	ppb	100
7) Acenaphthylene	5.63	152	49233	3.75096	ppb	99
8) Acenaphthene	5.83	154	12617	3.62921	ppb	99
9) Fluorene	6.42	166	14885	3.69482	ppb	98
11) Phenanthrene	7.52	178	19739	3.77915	ppb	100
12) Anthracene	7.57	178	18321	3.71376	ppb	100
14) Fluoranthene	8.89	202	32001	3.94391	ppb	99
16) Pyrene	9.14	202	32634	3.65012	ppb	99
17) Benz (a) anthracene	10.53	228	24722	3.77729	ppb	99
18) Chrysene	10.57	228	25985	3.57109	ppb	99
19) Indeno (1,2,3-cd) pyrene	14.28	276	18574	3.58954	ppb	# 94
21) Benzo (b) fluoranthene	12.02	252	23909	3.95214	ppb	97
22) Benzo (k) fluoranthene	12.07	252	25463	3.68068	ppb	99
23) Benzo (a) pyrene	12.60	252	21595	3.74776	ppb	99
24) Dibenz (a,h) anthracene	14.32	278	19960	3.50334	ppb	96
25) Benzo (g,h,i) perylene	14.58	276	22408	3.61398	ppb	95

Quantitation Report


Data File : M:\KYLO\DATA\211019\1019K440.D  
Acq On : 18 Nov 21 10:00  
Sample : 211115A LCSD-1 1/1000  
Misc :

Vial: 140  
Operator: LS  
Inst : KYLO  
Multiplr: 1.00

Quant Time: Nov 18 10:20 2021

Quant Results File: K1019.RES



Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)  
Title : EPA 8270  
Last Update : Tue Nov 30 08:16:15 2021  
Response via : Initial Calibration



Data File : M:\KYLO\DATA\211019\1019K001.D  
 Acq On : 19 Oct 21 13:58  
 Sample : SV TUNE 7/2/21  
 Misc :

Vial: 1  
 Operator: LS  
 Inst : KYLO  
 Multiplr: 1.00

Method : M:\KYLO\DATA\211019\DFTPP2.M (Chemstation Integrator)  
 Title :



AutoFind: Scans 476, 477, 478; Background Corrected with Scan 470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.8	44033	PASS
68	69	0.00	2	1.7	772	PASS
70	69	0.00	2	0.4	170	PASS
127	198	10	80	54.6	65376	PASS
197	198	0.00	2	0.2	185	PASS
198	198	100	100	100.0	119640	PASS
199	198	5	9	6.5	7734	PASS
275	198	10	60	23.2	27808	PASS
365	198	1	100	2.5	3043	PASS
441	442	0.01	24	13.9	12169	PASS
442	198	50	500	73.4	87760	PASS
443	442	15	24	18.4	16149	PASS

Data File Name: 1019K001.D  
Data File Path: M:\KYLO\DATA\211019\  
Operator: LS  
Date Acquired: 19 Oct 2021 13:58  
Method File: DFTPP2.M  
Sample Name: SV TUNE 7/2/21  
Vial Number: 1  
Instrument Name: KYLO



#	Name	Ret Time	Target Response
1)	DDT	7.36	16763500
2)	DDD	7.13	0
3)	DDE	6.80	0

Breakdown 0.00

Data File : M:\KYLO\DATA\211019\1019K436.D  
 Acq On : 18 Nov 21 8:49  
 Sample : SV TUNE 7/2/21  
 Misc :

Vial: 136  
 Operator: LS  
 Inst : KYLO  
 Multiplr: 1.00

Method : M:\KYLO\DATA\211019\K1019.M (RTE Integrator)  
 Title : EPA 8270



AutoFind: Scans 447, 448, 449; Background Corrected with Scan 441

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.3	33215	PASS
68	69	0.00	2	1.5	562	PASS
70	69	0.00	2	0.5	189	PASS
127	198	10	80	52.8	54210	PASS
197	198	0.00	2	0.3	333	PASS
198	198	100	100	100.0	102699	PASS
199	198	5	9	6.7	6887	PASS
275	198	10	60	23.0	23627	PASS
365	198	1	100	2.4	2468	PASS
441	442	0.01	24	13.9	10754	PASS
442	198	50	500	75.4	77456	PASS
443	442	15	24	18.2	14130	PASS

Data File Name: 1019K436.D  
Data File Path: M:\KYLO\DATA\211019\  
Operator: LS  
Date Acquired: 18 Nov 2021 08:49  
Method File: DFTPP2.M  
Sample Name: SV TUNE 7/2/21  
Vial Number: 136  
Instrument Name: KYLO

#	Name	Ret Time	Target Response
1)	DDT	7.12	13432000
2)	DDD	6.78	0
3)	DDE	6.57	0

Breakdown 0.00

Name of Final Standard

SIM Curve

Prep'd By (Initials)

LS

Prep Date

10/13/2021

Exp Date

6/17/2022

Initial Standard Information						Final Standard Information			
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc. (range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
1.0 ug/mL SIM	APPL	1.0 ug/mL SIM	1.0 ug/mL	9/9/2021	6/17/2022	10 uL	100uL	MC 61117 90uL	0.1 ug/mL
SIM Internal Standard	APPL	SIM Internal Standard	125 ug/mL	6/17/2021	6/17/2022	2 uL	*	*	2.5ug/mL
1.0 ug/mL SIM	APPL	1.0 ug/mL SIM	1.0 ug/mL	9/9/2021	6/17/2022	20 uL	100uL	MC 61117 80uL	0.2 ug/mL
SIM Internal Standard	APPL	SIM Internal Standard	125 ug/mL	6/17/2021	6/17/2022	2 uL	*	*	2.5ug/mL
5.0 ug/mL SIM	APPL	5.0 ug/mL SIM	5.0 ug/mL	9/9/2021	6/17/2022	10 uL	100uL	MC 61117 90uL	0.5 ug/mL
SIM Internal Standard	APPL	SIM Internal Standard	125 ug/mL	6/17/2021	6/17/2022	2 uL	*	*	2.5ug/mL
5.0 ug/mL SIM	APPL	5.0 ug/mL SIM	5.0 ug/mL	9/9/2021	6/17/2022	20 uL	100uL	MC 61117 80 uL	1.0 ug/mL
SIM Internal Standard	APPL	SIM Internal Standard	125 ug/mL	6/17/2021	6/17/2022	2 uL	*	*	2.5ug/mL
SIM STOCK	APPL	SIM STOCK	200 ug/mL	6/17/2021	6/17/2022	5 uL	200uL	MC 61117 190 uL	5.0 ug/mL
SIM SURROGATE	APPL	SIM SURR	100 ug/mL	6/17/2021	6/17/2022	5 uL	*	*	2.5ug/mL
SIM Internal Standard	APPL	SIM Internal Standard	125 ug/mL	6/17/2021	6/17/2022	4 uL	*	*	2.5ug/mL
SIM STOCK	APPL	SIM STOCK	200 ug/mL	6/17/2021	6/17/2022	5 uL	100 uL	MC 61117 90 uL	10 ug/mL
SIM SURROGATE	APPL	SIM SURR	100 ug/mL	6/17/2021	6/17/2022	5 uL	*	*	5 ug/mL
SIM Internal Standard	APPL	SIM Internal Standard	125 ug/mL	6/17/2021	6/17/2022	2 uL	*	*	2.5ug/mL
SIM STOCK	APPL	SIM STOCK	200 ug/mL	6/17/2021	6/17/2022	25 uL	100uL	MC 61117 50 uL	50 ug/mL
SIM SURROGATE	APPL	SIM SURR	100 ug/mL	6/17/2021	6/17/2022	25 uL	*	*	25 ug/mL
SIM Internal Standard	APPL	SIM Internal Standard	125 ug/mL	6/17/2021	6/17/2022	2 uL	*	*	2.5ug/mL
SIM STOCK	APPL	SIM STOCK	200 ug/mL	6/17/2021	6/17/2022	50 uL	100uL	na	100 ug/mL
SIM SURROGATE	APPL	SIM SURR	100 ug/mL	6/17/2021	6/17/2022	50 uL	*	*	50 ug/mL
SIM Internal Standard	APPL	SIM Internal Standard	125 ug/mL	6/17/2021	6/17/2022	2 uL	*	*	2.5ug/mL

Name of Final Standard

8270 PAH SIM Second Source

Prep'd By (Initials)

LS

Prep Date

10/13/2021

Exp Date

6/17/2022

Initial Standard Information						Final Standard Information			
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc. (range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
PAH SIM SS Stock	Phenova	AL0-130490	200 ug/mL	6/17/2021	6/17/2022	5 uL	200uL	MC 61117 195uL	5 ug/mL
SIM Internal Standard	APPL	SIM Internal Standard	125 ug/mL	6/17/2021	6/17/2022	4 uL	*	*	2.5ug/mL



Name of Final Standard PAH SIM Stock (Ampule)  
 Prep Date 6/17/2021  
 Exp Date 6/17/2022

Prep'd By (Initials) LS

Initial Standard Information					Final Standard Information				
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc.(range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
Custom PAH SIM Mix	Phenova	ALO-130490	200 ug/mL	CL13121-52443	12/31/2022	1000 uL	1mL	NA	200 ug/mL

Name of Final Standard SIM Surrogate  
 Prep Date 6/17/2021  
 Exp Date 6/17/2022

Prep'd By (Initials) LS

Initial Standard Information					Final Standard Information				
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc.(range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
Sim Surrogate Deuterated	Restek	33913	2000 ug/mL	A0161454-50793	5/31/2026	1 mL	20 mL	Acetone #0246130	100 ug/mL

Name of Final Standard 8270 SIM PAH Internal Standard  
 Prep Date 6/17/2021  
 Exp Date 6/17/2022

Prep'd By (Initials) LS

Initial Standard Information					Final Standard Information				
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc.(range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
SV Internal Standard	Restek	31206	2000 ug/mL	A0162879-50593	6/30/2026	625uL	10mL	MC 60338	125 ug/mL

Name of Final Standard SIM SS Stock (Ampule second source)  
 Prep Date 6/17/2021  
 Exp Date 6/17/2022

Prep'd By LS

Initial Standard Information					Final Standard Information				
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc.(range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
Custom PAH SIM Mix	Phenova	ALO-130490	200 ug/mL	CL13117-51757	12/31/2022	1000 uL	1mL	NA	200 ug/mL

Name of Final Standard PAH SIM Stock (Ampule)  
 Prep Date 6/17/2021  
 Exp Date 6/17/2022

Prep'd By (Initials) LS

Initial Standard Information						Final Standard Information			
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc.(range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
Custom PAH SIM Mix	Phenova	ALO-130490	200 ug/mL	CL13121-52443	12/31/2022	1000 uL	1mL	NA	200 ug/mL

Name of Final Standard SIM Surrogate  
 Prep Date 6/17/2021  
 Exp Date 6/17/2022

Prep'd By (Initials) LS

Initial Standard Information						Final Standard Information			
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc.(range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
Sim Surrogate Deuterated	Restek	33913	2000 ug/mL	A0161454-50793	5/31/2026	1 mL	20 mL	Acetone #0246130	100 ug/mL

Name of Final Standard 8270 SIM PAH Internal Standard  
 Prep Date 6/17/2021  
 Exp Date 6/17/2022

Prep'd By (Initials) LS

Initial Standard Information						Final Standard Information			
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc.(range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
SV Internal Standard	Restek	31206	2000 ug/mL	A0162879-50593	6/30/2026	625uL	10mL	MC 60338	125 ug/mL

Name of Final Standard SIM SS Stock (Ampule second source)  
 Prep Date 6/17/2021  
 Exp Date 6/17/2022

Prep'd By LS

Initial Standard Information						Final Standard Information			
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc.(range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
Custom PAH SIM Mix	Phenova	ALO-130490	200 ug/mL	CL13117-51757	12/31/2022	1000 uL	1mL	NA	200 ug/mL

Name of Final Standard 5 SIM CCV (2x)  
 Prep Date 10/19/2021  
 Exp Date 6/17/2022

Prep'd By (Initials) LS

Initial Standard Information						Final Standard Information			
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc.(range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot#.(or APPL Prep Date)	Final Standard Conc (range)
SIM STOCK	APPL	SIM STOCK	200 ug/mL	6/17/2021	12/31/2022	5 uL	200uL	MC 61117 190 uL	5.0 ug/mL
SIM SURROGATE	APPL	SIM SURR	100 ug/mL	6/17/2021	5/31/2026	5 uL	*	*	2.5ug/mL
SIM Internal Standard	APPL	SIM Internal Standard	125 ug/mL	6/17/2021	6/30/2026	4 uL	*	*	2.5ug/mL

Name of Final Standard SIM Surrogate  
 Prep Date 9/21/2021  
 Exp Date 9/21/2022

Prep'd By (Initials) LS/IC

Initial Standard Information						Final Standard Information			
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc. (range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
Sim Surrogate Deuterated	Restek	33913	2000 ug/mL	A0173323-52639	5/31/2027	1 mL	20 mL	Acetone #0246130	100 ug/mL

Name of Final Standard SIM Surrogate  
 Prep Date 8/24/2021  
 Exp Date 8/24/2022

Prep'd By (Initials) LS

Initial Standard Information						Final Standard Information			
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc.(range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Allquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
Sim Surrogate Deuterated	Restek	33913	2000 ug/mL	A0173323-52640	5/31/2027	1 mL	20 mL	Acetone #0246130	100 ug/mL

Name of Final Standard SIM Spike  
 Prep Date 8/5/2021  
 Exp Date 5/28/2022

Prep'd By (Initials) LS

Initial Standard Information						Final Standard Information			
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc.(range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
Custom PAH Sim Mix	Phenova	AL0-130490	200 ug/mL	CL13121- 50766,50767,50771,52444,52 445	5/28/2022	5 mL	25 mL	Acetone 0246130	40 ug/mL

Name of Final Standard 5 SIM CCV (2x)  
 Prep Date 10/19/2021  
 Exp Date 6/17/2022

Prep'd By (Initials) LS

Initial Standard Information						Final Standard Information			
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc.(range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
SIM STOCK	APPL	SIM STOCK	200 ug/mL	6/17/2021	12/31/2022	5 uL	200uL	MC 61117 190 uL	5.0 ug/mL
SIM SURROGATE	APPL	SIM SURR	100 ug/mL	6/17/2021	5/31/2026	5 uL	*	*	2.5ug/mL
SIM Internal Standard	APPL	SIM Internal Standard	125 ug/mL	6/17/2021	6/30/2026	4 uL	*	*	2.5ug/mL

Name of Final Standard SIM Surrogate  
 Prep Date 8/24/2021  
 Exp Date 8/24/2022

Prep'd By (Initials) LS

Initial Standard Information						Final Standard Information			
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc.(range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
Sim Surrogate Deuterated	Restek	33913	2000 ug/mL	A0173323-52640	5/31/2027	1 mL	20 mL	Acetone #0246130	100 ug/mL



Name of Final Standard SIM Surrogate  
 Prep Date 9/21/2021  
 Exp Date 9/21/2022

Prep'd By (Initials) LS/C

Initial Standard Information						Final Standard Information			
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc.(range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
Sim Surrogate Deuterated	Restek	33913	2000 ug/mL	A0173323-52639	5/31/2027	1 mL	20 mL	Acetone #0246130	100 ug/mL

# Organic Extraction Worksheet

<b>Method</b>	Continuous Liquid/Liquid SVOC 3520C	<b>Extraction Set</b>	211115A	<b>Extraction Method</b>	LIQ003	<b>Units</b>	mL
<b>Spiked ID 1</b>	Sim Spike 10-21-21 10-21-22	<b>Surrogate ID 1</b>	SIM Surrogate 10-21-21 10-21-22				
<b>Spiked ID 2</b>		<b>Surrogate ID 2</b>					
<b>Spiked ID 3</b>		<b>Surrogate ID 3</b>					
<b>Spiked ID 4</b>		<b>Surrogate ID 4</b>					
<b>Spiked ID 5</b>		<b>Surrogate ID 5</b>					
<b>Spiked ID 6</b>		<b>Sufficient Vol for Matrix QC:</b>		NO			
<b>Spiked ID 7</b>		<b>Ext. Start Time:</b>		11/15/21 13:18			
<b>Spiked ID 8</b>		<b>Ext. End Time:</b>		11/16/21 7:19			
<b>GC Requires Extract By:</b>							
pH1	14	11/15/21 10:37	Water Bath Temp 1 °C	75/74.5 E-WB5 °			
pH2	14	11/16/21 10:25	Water Bath Temp 2 °C				
pH3			Water Bath Temp 3 °C				

Spiked By: SR

Date 11/15/2021

Witnessed By: CG

Date 11/15/2021

Sample	Sample Container	Spike Amount	Spike ID	Surrogate Amount	Surrogate ID	Extract Amount	Final Volume	pH	Extract Date/Time	Comments
1	211115A Blk			0.050	1	1000	1	14	11/15/21 10:23	
					equip	E-HP15 E-WB5				
2	211115A LCS-1	0.125	1	0.050	1	1000	1	14	11/15/21 10:23	
					equip	E-HP16 E-WB5				
3	211115A LCSD-1	0.125	1	0.050	1	1000	1	14	11/15/21 10:23	
					equip	E-HP17 E-WB5				
4	BA45998 BA45998W09			0.050	1	1000	1	14	11/15/21 10:23	98209
					equip	E-HP19 E-WB5				
5	BA46001 BA46001W07			0.050	1	1000	1	14	11/15/21 10:23	98213
					equip	E-HP20 E-WB5				
6	BA46103 BA46103W07			0.050	1	950	1	14	11/15/21 10:23	98214
					equip	E-HP21 E-WB5				
7	BA46105 BA46105W07			0.050	1	1050	1	14	11/15/21 10:23	98214
					equip	E-HP13 E-WB5				
8	BA46107 BA46107W07			0.050	1	1030	1	14	11/15/21 10:23	98214
					equip	E-HP23 E-WB5				
9	BA46109 BA46109W07			0.050	1	1000	1	14	11/15/21 10:23	98214 Extractor broke lost extract redo
					equip	E-HP24 E-WB5				
10	BA46109 (DUP) BA46109W08			0.050	1	1000	1	14	11/16/21 10:20	98214 RE-DO
					equip	E-HP15 E-WB5				
11	BA46115 BA46115W07			0.050	1	1000	1	14	11/15/21 10:23	98212
					equip	E-HP16 E-WB5				
12	BA46116 BA46116W05			0.050	1	1000	1	14	11/15/21 10:23	98212
					equip	E-HP17 E-WB5				
13	BA46117 BA46117W02			0.050	1	1010	1	14	11/15/21 10:23	98212
					equip	E-HP19 E-WB5				

<b>Solvent and Lot#</b>	
PH Strips	HC155968
Dichloromethane (DCM)	61117
10N NaO (10mLs)	10-17-21
Filter Paper	400202
Na2SO4	2021071206

<b>Extraction COC Transfer</b>	
Extraction lab employee Initials	KY
GC analyst's initials	LS
Date	11/18/21
Time	0813
Refrigerator	GC_C

<b>Technician's Initials</b>	
Scanned By	SR
Sample Preparation	SR
Extraction	SR
Concentration	SR
Modified	11/18/2021 6:54:19 AM

Reviewed By: KY

Date 11/18/2021

## Injection Log

Directory: M:\KYLO\DATA\211019\

Line	Vial	FileName	Multiplier	SampleName	Misc Info	Injected
1	1	1019K001.D	1	SV TUNE 7/2/21		19 Oct 21 13:58
2	2	1019K002.D	1	0.1 ug/ml 10/13/21		19 Oct 21 14:09
3	3	1019K003.D	1	0.2 ug/ml 10/13/21		19 Oct 21 14:29
4	4	1019K004.D	1	0.5 ug/ml 10/13/21		19 Oct 21 14:49
5	5	1019K005.D	1	1 ug/ml 10/13/21		19 Oct 21 15:09
6	6	1019K006.D	1	5 ug/ml 10/13/21		19 Oct 21 15:29
7	7	1019K007.D	1	10 ug/ml 10/13/21		19 Oct 21 15:49
8	8	1019K008.D	1	50 ug/ml 10/13/21		19 Oct 21 16:09
9	9	1019K009.D	1	100 ug/ml 10/13/21		19 Oct 21 16:29
10	10	1019K010.D	1	SS ug/ml 10/13/21		19 Oct 21 16:49
11	136	1019K436.D	1	SV TUNE 7/2/21		18 Nov 21 8:49
12	137	1019K437.D	1	5 ug/ml 10/19/21 (1)		18 Nov 21 9:01
13	138	1019K438.D	1	211115A BLK 1/1000		18 Nov 21 9:21
14	139	1019K439.D	1	211115A LCS-1 1/1000		18 Nov 21 9:40
15	140	1019K440.D	1	211115A LCSD-1 1/1000		18 Nov 21 10:00
22	148	1019K448.D	1	BA46115W07 1/1000		18 Nov 21 12:40
23	149	1019K449.D	1	BA46116W05 1/1000		18 Nov 21 13:00
24	150	1019K450.D	0.990099	BA46117W02 1/1010		18 Nov 21 13:20
25	22	1019K472.D	1	5 ug/ml 10/13/21 (2)		18 Nov 21 20:38

**ORGANICS**  
**Calibration Data**

VOLATILE ORGANIC ANALYSIS  
VOLATILE ORGANIC COMPOUNDS

**Form 6**  
**Initial Calibration**

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Initial Cal. Date: 11/9/2021  
Instrument: Thor

Initials:   MH  

1109T14.D    1109T15.D    1109T16.D    1109T17.D    1109T18.D    1109T19.D    1109T20.D    1109T21.D    1109T22.D

	Compound	1	2	3	4	5	6	7	8	9		Avg	%RSD	Type	r <sup>2</sup>	Q	MRF
1	I Fluorobenzene (IS)																
2	TM Chlorotrifluoroethene													TM			
3	TML Dichlorodifluoromethane	0.1010	0.0902	0.1163	0.0905	0.0775	0.0882	0.0726	0.0756			0.09	16	TM	0.998		
4	TMQ Freon 114	0.0190	0.0450	0.0418	0.0608	0.0638	0.0746	0.0642	0.0670			0.05	33	TM	0.998		
5	TM*L Chloromethane	0.0565	0.0405	0.0400	0.0287	0.0244	0.0281	0.0266	0.0269	0.0252		0.03	32	TM**	0.999		
6	TM*L Vinyl chloride	0.0940	0.0545	0.0612	0.0656	0.0627	0.0706	0.0664	0.0721	0.0683		0.07	16	TM*	0.999		
####	TML Bromomethane	0.0635	0.0812	0.0608	0.0704	0.0560	0.0562	0.0539	0.0547	0.0499		0.06	16	TM	0.999		
####	TML Chloroethane	0.0115	0.0141	0.0455	0.0471	0.0409	0.0420	0.0368	0.0378	0.0302		0.03	38	TM	0.990		
####	TML Dichlorofluoromethane	0.0721	0.1641	0.1635	0.1552	0.1321	0.1559	0.1440	0.1527	0.1276		0.14	20	TM	0.994		
####	TM Trichlorofluoromethane	0.2244	0.2133	0.2326	0.2668	0.2200	0.2531	0.2448	0.2627	0.2222		0.24	8.3	TM			
####	TM Acrolein	0.0098	0.0118	0.0128	0.0125	0.0124	0.0131	0.0137	0.0136	0.0119		0.01	9.5	TM			
####	TM Acetone	0.0198	0.0213	0.0223	0.0236	0.0246	0.0254	0.0250	0.0251	0.0242		0.02	8.2	TM			
####	TM Freon-113	0.0620	0.0645	0.0523	0.0660	0.0434	0.0536	0.0532	0.0588	0.0571		0.06	12	TM			
####	TM*L 1,1-DCE	0.1221	0.1381	0.1420	0.1542	0.1161	0.1518	0.1408	0.1465	0.1465		0.14	9.2	TM*	1.000		
####	TMQ Acetonitrile	0.0016	0.0015	0.0011	0.0012	0.0013	0.0011	0.0011	0.0010	0.0009		0.00	17	TM	0.992		
####	TM t-Butanol	0.0036	0.0031	0.0030	0.0034	0.0032	0.0032	0.0030	0.0028			0.00	8.3	TM			
####	TML Methyl Acetate			0.0234	0.0390	0.0302	0.0454	0.0475	0.0517	0.0546		0.04	28	TM	0.999		
####	TML Iodomethane	0.0781	0.0653	0.0619	0.0743	0.0522	0.0591	0.0536	0.0535			0.06	16	TM	0.999		
####	TML Acrylonitrile				0.0008	0.0081	0.0147	0.0195	0.0219	0.0229		0.01	59	TM	1.000		
####	TML Methylene chloride	0.0409	0.0870	0.0871	0.0831	0.0786	0.0996	0.0867	0.0973	0.0921		0.08	21	TM	0.999		
####	TML Carbon disulfide	0.1825	0.1164	0.1116	0.1458	0.1019	0.1206	0.1104	0.1142	0.1034		0.12	21	TM	0.998		
####	TM Methyl t-butyl ether (MtBE)	0.2306	0.2485	0.2682	0.2614	0.2269	0.2725	0.2659	0.2912	0.2969		0.26	9.2	TM			
####	TML Trans-1,2-DCE	0.0648	0.1027	0.0957	0.1103	0.1009	0.1231	0.1195	0.1290	0.1270		0.11	19	TM	1.000		
####	TML Diisopropyl Ether	0.0440	0.1532	0.1812	0.1722	0.1569	0.1907	0.1819	0.1985	0.2006		0.16	29	TM	1.000		
####	TM*L 1,1-DCA	0.0768	0.1347	0.1617	0.1381	0.1203	0.1510	0.1441	0.1631	0.1614		0.14	20	TM**	0.999		
####	TML Vinyl Acetate			0.0647	0.0806	0.0974	0.1409	0.1483	0.1840	0.1902		0.13	38	TM	0.992		
####	TM Ethyl tert Butyl Ether	0.2400	0.1525	0.2028	0.2303	0.2079	0.2448	0.2384	0.2602	0.2588		0.23	15	TM			

VOLATILE ORGANIC ANALYSIS  
VOLATILE ORGANIC COMPOUNDS

**Form 6**  
**Initial Calibration**

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Initial Cal. Date: 11/9/2021  
Instrument: Thor

Initials: MH

	Compound	1	2	3	4	5	6	7	8	9		Avg	%RSD	Type	Q	MRF
####	TM MEK (2-Butanone)	0.0208	0.0286	0.0294	0.0295	0.0299	0.0313	0.0333	0.0347	0.0339		0.03	14	TM		
####	TM Cis-1,2-DCE	0.0976	0.1111	0.1194	0.1400	0.1192	0.1460	0.1424	0.1527	0.1538		0.13	15	TM		
####	TM 2,2-Dichloropropane	0.1218	0.1455	0.1796	0.1887	0.1544	0.1809	0.1827	0.1991	0.1944		0.17	15	TM		
####	TM* Chloroform	0.1437	0.1818	0.1879	0.2205	0.1805	0.2325	0.2088	0.2281	0.2230		0.20	15	TM*		
####	TML Bromochloromethane		0.0296	0.0556	0.0567	0.0512	0.0619	0.0592	0.0606	0.0597		0.05	19	TM	1.000	
####	S Dibromofluoromethane(S)	0.2231	0.2208	0.2683	0.2711	0.2992	0.2972	0.3055	0.3176	0.3150		0.28	13	S		
####	TM 1,1,1-TCA	0.0955	0.1326	0.1053	0.0941	0.0861	0.1019	0.0988	0.1079	0.1064		0.10	13	TM		
####	TML Cyclohexane	0.0646	0.1124	0.1190	0.1338	0.0989	0.1342	0.1282	0.1435	0.1407		0.12	21	TM	1.000	
####	TML 1,1-Dichloropropene	0.0869	0.1337	0.1305	0.1479	0.1164	0.1423	0.1429	0.1505	0.1529		0.13	16	TM	1.000	
####	TM 2,2,4-Trimethylpentane	0.2442	0.2303	0.2804	0.2983	0.2310	0.2904	0.2827	0.3118	0.3119		0.28	12	TM		
####	S 1,2-DCA-D4(S)	0.2413	0.2497	0.2923	0.2850	0.3172	0.3123	0.3260	0.3344	0.3368		0.30	12	S		
####	TML Carbon Tetrachloride	0.1086	0.1768	0.2245	0.1987	0.1933	0.2276	0.2315	0.2536	0.2586		0.21	22	TM	1.000	
####	TM Tert Amyl Methyl Ether	0.2483	0.2678	0.2732	0.2749	0.2248	0.2807	0.2714	0.2993	0.2984		0.27	8.6	TM		
####	TML Methylcyclopentane				0.0045	0.0077	0.0112	0.0121	0.0114	0.0112		0.01	31	TM	0.999	
####	TM 1,2-DCA	0.2083	0.1712	0.1629	0.1598	0.1470	0.1638	0.1668	0.1763	0.1730		0.17	9.9	TM		
####	TM Benzene	0.4308	0.4049	0.4042	0.3936	0.3372	0.4005	0.3828	0.4105	0.4063		0.40	6.5	TM		
####	TM TCE	0.1216	0.0751	0.0941	0.0901	0.0760	0.0905	0.0891	0.0970	0.0991		0.09	15	TM		
####	TM 2-Pentanone	0.0658	0.0612	0.0605	0.0607	0.0627	0.0622	0.0635	0.0625	0.0569		0.06	3.9	TM		
####	TM* 1,2-Dichloropropane	0.0851	0.0794	0.0988	0.0899	0.0729	0.0966	0.0901	0.0984	0.0943		0.09	10.0	TM*		
####	TM Bromodichloromethane	0.1479	0.1660	0.1577	0.1751	0.1367	0.1634	0.1624	0.1815	0.1821		0.16	9.2	TM		
####	TM Methyl Cyclohexane	0.1406	0.1940	0.1924	0.1820	0.1446	0.1921	0.1888	0.2111	0.2061		0.18	14	TM		
####	TML Dibromomethane	0.0568	0.1676	0.1601	0.1494	0.1316	0.1586	0.1499	0.1659	0.1660		0.15	24	TM	1.000	
####	TM MIBK (methyl isobutyl ketone)	0.0693	0.0730	0.0755	0.0790	0.0823	0.0829	0.0847	0.0868	0.0902		0.08	8.4	TM		
####	TM 1-Bromo-2-chloroethane	0.0604	0.0762	0.0543	0.0645	0.0514	0.0663	0.0593	0.0651	0.0666		0.06	12	TM		
####	TM Cis-1,3-Dichloropropene	0.1424	0.1681	0.1697	0.1753	0.1303	0.1734	0.1720	0.1835	0.1869		0.17	11	TM		
####	TM* Toluene	0.5050	0.5592	0.5036	0.5408	0.4374	0.5429	0.5102	0.5538	0.5464		0.52	7.3	TM*		
####	TM Trans-1,3-Dichloropropene	0.1565	0.1572	0.1394	0.1668	0.1356	0.1627	0.1656	0.1849	0.1859		0.16	11	TM		
####	TML 1,1,2-TCA	0.0570	0.1066	0.1217	0.1157	0.0971	0.1107	0.1089	0.1177	0.1171		0.11	19	TM	1.000	
####	TM 2-Hexanone	0.0456	0.0510	0.0505	0.0561	0.0574	0.0586	0.0595	0.0635	0.0648		0.06	11	TM		
####	I Chlorobenzene-D5 (IS)															
####	S Toluene-D8(S)	0.8367	0.8086	0.9421	0.9532	1.035	1.030	1.053	1.098	1.092		0.98	11	S		
####	TM 1,2-EDB	0.1167	0.1106	0.1234	0.1330	0.1160	0.1427	0.1296	0.1450	0.1456		0.13	10	TM		

VOLATILE ORGANIC ANALYSIS  
VOLATILE ORGANIC COMPOUNDS

Form 6  
Initial Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Initial Cal. Date: 11/9/2021  
Instrument: Thor

Initials: MH

	Compound	1	2	3	4	5	6	7	8	9		Avg	%RSD	Type	Q	MRF
####	TM Tetrachloroethene	0.3304	0.2617	0.2675	0.2778	0.2356	0.2865	0.2663	0.2987	0.2893		0.28	9.5	TM		
####	TML 1-Chlorohexane	0.1644	0.2405	0.2476	0.1829	0.1544	0.1861	0.1757	0.1906	0.1893		0.19	16	TM	1.000	
####	TM 1,1,1,2-Tetrachloroethane	0.1701	0.1668	0.1822	0.1819	0.1551	0.1901	0.1746	0.2000	0.1984		0.18	8.3	TM		
####	TM m&p-Xylene	0.4684	0.4797	0.4932	0.4864	0.4466	0.5397	0.5097	0.5573	0.5439		0.50	7.5	TM		
####	TM o-Xylene	0.6118	0.5243	0.5206	0.4971	0.4373	0.5493	0.5111	0.5595	0.5550		0.53	9.1	TM		
####	TM Styrene	0.3514	0.3750	0.3584	0.3801	0.3282	0.4250	0.4019	0.4487	0.4467		0.39	11	TM		
####	S 4-Bromofluorobenzene(S)	0.3341	0.3113	0.3679	0.3753	0.4120	0.4174	0.4327	0.4458	0.4350		0.39	12	S		
####	TM 1,3-Dichloropropane	0.1525	0.1520	0.1731	0.1657	0.1509	0.1768	0.1629	0.1801	0.1798		0.17	7.3	TM		
####	TM Dibromochloromethane	0.1838	0.1648	0.1729	0.1723	0.1528	0.1821	0.1745	0.1976	0.1996		0.18	8.4	TM		
####	TM** Chlorobenzene	0.5274	0.4353	0.4219	0.4437	0.3758	0.4533	0.4134	0.4546	0.4487		0.44	9.2	TM**		
####	TM* Ethylbenzene	0.7312	0.6661	0.6395	0.6455	0.5415	0.6664	0.6209	0.6954	0.6800		0.65	8.1	TM*		
####	TM** Bromoform	0.1687	0.1364	0.1924	0.1759	0.1322	0.1826	0.1684	0.1971	0.1960		0.17	14	TM**		
####	I 1,4-Dichlorobenzene-D (IS)															
####	TM Isopropylbenzene	1.012	0.9400	0.9529	0.9360	0.8093	1.041	1.008	1.088	1.082		0.99	8.8	TM		
####	TM** 1,1,2,2-Tetrachloroethane	0.1783	0.1997	0.1819	0.1796	0.1744	0.2121	0.2004	0.2191	0.2161		0.20	9.0	TM**		
####	TML 1,2,3-Trichloropropane	0.0790	0.0618	0.1140	0.0905	0.0672	0.0925	0.0847	0.0951	0.0916		0.09	18	TM	0.999	
####	TML t-1,4-Dichloro-2-Butene			0.0148	0.0482	0.0345	0.0546	0.0433	0.0519	0.0564		0.04	34	TM	0.998	
####	TM Bromobenzene	0.3254	0.3828	0.3566	0.3717	0.3115	0.3733	0.3570	0.3930	0.3862		0.36	7.7	TM		
####	TM n-Propylbenzene	1.129	1.102	1.041	1.089	0.8961	1.113	1.065	1.169	1.161		1.1	7.6	TM		
####	TM 4-Ethyltoluene	1.126	1.026	0.9187	0.9518	0.8188	1.045	1.006	1.088	1.080		1.0	9.6	TM		
####	TM 2-Chlorotoluene	0.7901	0.6488	0.7561	0.7327	0.6306	0.7745	0.7275	0.8089	0.7847		0.74	8.4	TM		
####	TM 1,3,5-Trimethylbenzene	1.094	0.8706	0.8782	0.8349	0.7404	0.9049	0.8727	0.9504	0.9318		0.90	11	TM		
####	TM 4-Chlorotoluene	0.6965	0.7089	0.7491	0.7385	0.6518	0.7852	0.7746	0.8274	0.8112		0.75	7.6	TM		
####	TM Tert-Butylbenzene	1.034	0.7729	0.9343	0.9476	0.7876	0.9668	0.9567	1.011	1.000		0.93	10.0	TM		
####	TM 1,2,4-Trimethylbenzene	0.8578	0.8896	0.8020	0.8181	0.6852	0.8967	0.8648	0.9470	0.9318		0.85	9.3	TM		
####	TM Sec-Butylbenzene	1.290	0.9998	0.9707	1.056	0.8756	1.118	1.076	1.164	1.164		1.1	11	TM		
####	TM p-Isopropyltoluene	1.132	0.9485	0.9365	0.9814	0.8631	1.067	1.034	1.133	1.110		1.0	9.4	TM		
####	TM Benzyl Chloride	0.3351	0.3677	0.3404	0.3580	0.3447	0.3943	0.3932	0.4507	0.4704		0.38	13	TM		
####	TM 1,3-DCB	0.8014	0.6985	0.6038	0.6349	0.5416	0.6590	0.6428	0.6881	0.6728		0.66	11	TM		
####	TM 1,4-DCB	0.8748	0.6985	0.6811	0.6501	0.5758	0.6670	0.6308	0.6901	0.6717		0.68	12	TM		
####	TM n-Butylbenzene	0.6815	0.6350	0.6636	0.7157	0.6113	0.7647	0.7514	0.8183	0.8315		0.72	11	TM		
####	TM 1,2-DCB	0.7382	0.6026	0.5723	0.5748	0.4739	0.6203	0.5811	0.6396	0.6319		0.60	12	TM		
####	TML Hexachloroethane	0.1280	0.1211	0.2092	0.2382	0.2248	0.2554	0.2567	0.2854	0.2970		0.22	28	TM	0.999	
####	TML 1,2-Dibromo-3-chloropropane	0.0174	0.0263	0.0477	0.0625	0.0586	0.0695	0.0718	0.0832	0.0900		0.06	42	TM	0.998	
####	TML 1,2,4-Trichlorobenzene	0.5875	0.4360	0.4012	0.4237	0.3580	0.4775	0.4601	0.5182	0.5490		0.47	16	TM	0.999	

Data File : M:\THOR\DATA\211109\1109T14.D  
 Acq On : 9 Nov 21 11:48  
 Sample : 0.3ug/L VOC STD 11/9/21  
 Misc : IS&S 8/15/21

Vial: 2  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 10 9:44 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 09:43:41 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.35	96	320118	25.00	ppb	0.00
68) Chlorobenzene-D5 (IS)	9.81	117	309209	25.00	ppb	0.00
83) 1,4-Dichlorobenzene-D (IS)	12.37	152	205673	25.00	ppb	0.00
System Monitoring Compounds						
43) Dibromofluoromethane(S)	5.50	111	14281	4.25	ppb	0.00
Spiked Amount	25.000		Recovery	=	16.996%	
48) 1,2-DCA-D4(S)	5.91	65	15450	4.63	ppb	0.00
Spiked Amount	25.000		Recovery	=	18.512%	
69) Toluene-D8(S)	8.22	98	51740	4.11	ppb	0.00
Spiked Amount	25.000		Recovery	=	16.436%	
77) 4-Bromofluorobenzene(S)	11.11	95	20661	4.24	ppb	0.00
Spiked Amount	25.000		Recovery	=	16.976%	
Target Compounds						
3) Dichlorodifluoromethane	1.09	85	388	-1.65	ppb #	45
4) Freon 114	1.20	85	73	-0.78	ppb #	58
5) Chloromethane	1.29	50	217	0.49	ppb #	42
6) Vinyl chloride	1.33	62	361	0.32	ppb #	40
9) Bromomethane	1.60	96	244	0.31	ppb #	82
10) Chloroethane	1.68	64	44	0.08	ppb #	48
11) Dichlorofluoromethane	1.87	67	277	0.14	ppb #	39
12) Trichlorofluoromethane	1.92	101	862	0.34	ppb #	81
16) Acrolein	2.32	56	1257	7.82	ppb #	66
17) Acetone	2.50	43	1270	3.93	ppb #	50
18) Freon-113	2.42	101	238	0.36	ppb #	49
19) 1,1-DCE	2.41	61	469	0.20	ppb #	55
21) Acetonitrile	2.83	40	205	11.44	ppb #	51
22) t-Butanol	3.18	59	459	12.53	ppb #	57
26) Methylene chloride	2.96	49	157	-0.11	ppb #	63
27) Carbon disulfide	2.62	76	701	0.45	ppb #	74
28) Methyl t-butyl ether (MtBE)	3.35	73	886	0.26	ppb #	56
29) Trans-1,2-DCE	3.33	61	249	0.16	ppb #	73
33) 1,1-DCA	3.92	63	295	0.14	ppb #	50
35) Ethyl tert Butyl Ether	4.68	59	922	0.28	ppb #	73
36) MEK (2-Butanone)	4.91	43	1334	2.92	ppb #	86
37) Cis-1,2-DCE	4.83	61	375	0.19	ppb #	72
38) 2,2-Dichloropropane	4.78	77	468	0.22	ppb #	56
39) 2-Methylpentane	3.19	43	19	0.07	ppb #	9
41) Chloroform	5.29	83	552	0.21	ppb #	86
44) 1,1,1-TCA	5.49	97	367	0.33	ppb #	72
45) Cyclohexane	5.56	56	248	0.13	ppb #	67

(#) = qualifier out of range (m) = manual integration  
 1109T14.D T1109W.M Thu Nov 11 11:38:39 2021



Data File : M:\THOR\DATA\211109\1109T14.D  
 Acq On : 9 Nov 21 11:48  
 Sample : 0.3ug/L VOC STD 11/9/21  
 Misc : IS&S 8/15/21

Vial: 2  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 10 9:44 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 09:43:41 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
46) 1,1-Dichloropropene	5.73	75	334	0.18	ppb	# 36
47) 2,2,4-Trimethylpentane	6.14	57	938	0.23	ppb	# 61
49) Carbon Tetrachloride	5.70	117	417	0.18	ppb	# 34
50) Tert Amyl Methyl Ether	6.20	73	954	0.26	ppb	# 51
52) 1,2-DCA	6.02	62	800	0.41	ppb	# 73
53) Benzene	5.98	78	1655	0.30	ppb	# 92
54) TCE	6.80	130	467	0.44	ppb	# 77
55) 2-Pentanone	7.07	43	8425	9.45	ppb	# 93
56) 1,2-Dichloropropane	7.05	63	327	0.23	ppb	# 84
57) Bromodichloromethane	7.39	83	568	0.28	ppb	# 71
58) Methyl Cyclohexane	7.02	83	540	0.22	ppb	# 79
59) Dibromomethane	7.19	174	218	0.14	ppb	# 46
60) MIBK (methyl isobutyl ket	8.12	43	4438	3.61	ppb	# 98
61) 1-Bromo-2-chloroethane	7.74	63	232	0.24	ppb	# 48
63) Cis-1,3-Dichloropropene	7.93	75	547	0.24	ppb	# 71
64) Toluene	8.30	91	1940	0.28	ppb	# 90
65) Trans-1,3-Dichloropropene	8.56	75	601	0.29	ppb	# 61
66) 1,1,2-TCA	8.75	97	219	0.15	ppb	# 69
67) 2-Hexanone	9.06	43	2921	3.44	ppb	# 91
70) 1,2-EDB	9.29	107	433	0.26	ppb	# 77
71) Tetrachloroethene	8.90	166	1226	0.42	ppb	# 81
72) 1-Chlorohexane	9.85	91	610	0.25	ppb	# 84
73) 1,1,1,2-Tetrachloroethane	9.94	131	631	0.31	ppb	# 93
74) m&p-Xylene	10.11	91	3476	0.89	ppb	# 70
75) o-Xylene	10.54	91	2270	0.35	ppb	# 88
76) Styrene	10.56	104	1304	0.25	ppb	# 83
78) 1,3-Dichloropropane	8.93	76	566	0.24	ppb	# 40
79) Dibromochloromethane	9.18	129	682	0.33	ppb	# 88
80) Chlorobenzene	9.85	112	1957	0.36	ppb	# 90
81) Ethylbenzene	9.98	91	2713	0.33	ppb	# 91
82) Bromoform	10.75	173	626	0.35	ppb	# 36
84) Isopropylbenzene	10.95	105	2497	0.28	ppb	# 77
85) 1,1,2,2-Tetrachloroethane	11.27	83	440	0.22	ppb	# 72
86) 1,2,3-Trichloropropane	11.32	110	195	0.27	ppb	# 17
88) Bromobenzene	11.26	156	803	0.28	ppb	# 75
89) n-Propylbenzene	11.40	91	2786	0.28	ppb	# 91
90) 4-Ethyltoluene	11.53	105	2778	0.32	ppb	# 91
91) 2-Chlorotoluene	11.49	91	1950	0.29	ppb	# 83
92) 1,3,5-Trimethylbenzene	11.59	105	2701	0.36	ppb	# 98
93) 4-Chlorotoluene	11.61	91	1719	0.25	ppb	# 92
94) Tert-Butylbenzene	11.95	119	2551	0.32	ppb	# 90
95) 1,2,4-Trimethylbenzene	12.01	105	2117	0.29	ppb	# 93

(#) = qualifier out of range (m) = manual integration  
 1109T14.D T1109W.M Thu Nov 11 11:38:39 2021

Data File : M:\THOR\DATA\211109\1109T14.D  
 Acq On : 9 Nov 21 11:48  
 Sample : 0.3ug/L VOC STD 11/9/21  
 Misc : IS&S 8/15/21

Vial: 2  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 10 9:44 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 09:43:41 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
96) Sec-Butylbenzene	12.19	105	3185	0.34	ppb	97
97) p-Isopropyltoluene	12.35	119	2794	0.33	ppb #	87
98) Benzyl Chloride	12.55	91	827	0.23	ppb #	92
99) 1,3-DCB	12.30	146	1978	0.38	ppb	92
100) 1,4-DCB	12.39	146	2159	0.40	ppb #	86
101) n-Butylbenzene	12.81	91	1682	0.25	ppb #	78
102) 1,2-DCB	12.81	146	1822	0.38	ppb	97
103) Hexachloroethane	13.08	201	316	0.18	ppb #	70
104) 1,2-Dibromo-3-chloropropan	13.64	157	43	0.08	ppb #	15
105) 1,2,4-Trichlorobenzene	14.57	180	1450	0.43	ppb	95
106) Hexachlorobutadiene	14.76	225	1014	0.49	ppb #	56
107) Naphthalene	14.84	128	1128	0.37	ppb	98
108) 1,2,3-Trichlorobenzene	15.09	180	1232	0.39	ppb	86

Quantitation Report


Data File : M:\THOR\DATA\211109\1109T14.D  
Acq On : 9 Nov 21 11:48  
Sample : 0.3ug/L VOC STD 11/9/21  
Misc : IS&S 8/15/21

Vial: 2  
Operator:  
Inst : Thor  
Multiplr: 1.00

Quant Time: Nov 10 9:44 2021

Quant Results File: T1109W.RES

Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Wed Nov 10 10:21:13 2021  
Response via : Initial Calibration



Data File : M:\THOR\DATA\211109\1109T15.D  
 Acq On : 9 Nov 21 12:13  
 Sample : 0.5ug/L VOC STD 11/9/21  
 Misc : IS&S 8/15/21

Vial: 3  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 10 9:44 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 09:43:41 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.35	96	311081	25.00	ppb	0.00
68) Chlorobenzene-D5 (IS)	9.81	117	300686	25.00	ppb	0.00
83) 1,4-Dichlorobenzene-D (IS)	12.37	152	205596	25.00	ppb	0.00
<b>System Monitoring Compounds</b>						
43) Dibromofluoromethane (S)	5.50	111	13736	4.21	ppb	0.00
Spiked Amount	25.000		Recovery	=	16.824%	
48) 1,2-DCA-D4 (S)	5.91	65	15534	4.79	ppb	0.00
Spiked Amount	25.000		Recovery	=	19.152%	
69) Toluene-D8 (S)	8.22	98	48627	3.97	ppb	0.00
Spiked Amount	25.000		Recovery	=	15.884%	
77) 4-Bromofluorobenzene (S)	11.11	95	18718	3.95	ppb	0.00
Spiked Amount	25.000		Recovery	=	15.816%	
<b>Target Compounds</b>						
3) Dichlorodifluoromethane	1.09	85	561	-1.37	ppb	95
4) Freon 114	1.20	85	280	-0.48	ppb	80
5) Chloromethane	1.27	50	252	0.58	ppb	# 42
6) Vinyl chloride	1.33	62	339	0.31	ppb	# 71
7) Butane	1.59	43	43	41.62	ppb	# 100
9) Bromomethane	1.60	96	505	0.66	ppb	# 56
10) Chloroethane	1.68	64	88	0.16	ppb	# 48
11) Dichlorofluoromethane	1.87	67	1021	0.53	ppb	# 73
12) Trichlorofluoromethane	1.91	101	1327	0.54	ppb	# 89
16) Acrolein	2.32	56	3680	23.56	ppb	# 99
17) Acetone	2.49	43	2651	8.45	ppb	# 87
18) Freon-113	2.43	101	401	0.62	ppb	# 82
19) 1,1-DCE	2.41	61	859	0.44	ppb	# 91
21) Acetonitrile	2.81	40	458	25.29	ppb	# 72
22) t-Butanol	3.17	59	969	27.22	ppb	# 95
24) Iodomethane	2.55	142	406	0.17	ppb	# 81
26) Methylene chloride	2.96	49	541	0.20	ppb	# 38
27) Carbon disulfide	2.61	76	724	0.48	ppb	# 86
28) Methyl t-butyl ether (MtBE)	3.34	73	1546	0.47	ppb	# 94
29) Trans-1,2-DCE	3.33	61	639	0.41	ppb	# 62
31) Diisopropyl Ether	4.13	45	953	0.32	ppb	# 67
33) 1,1-DCA	3.92	63	838	0.42	ppb	# 76
35) Ethyl tert Butyl Ether	4.67	59	949	0.29	ppb	# 82
36) MEK (2-Butanone)	4.89	43	3556	8.01	ppb	# 81
37) Cis-1,2-DCE	4.82	61	691	0.36	ppb	# 91
38) 2,2-Dichloropropane	4.80	77	905	0.43	ppb	# 56
39) 2-Methylpentane	3.16	43	343	1.33	ppb	# 23

(#) = qualifier out of range (m) = manual integration  
 1109T15.D T1109W.M Thu Nov 11 11:38:41 2021

Data File : M:\THOR\DATA\211109\1109T15.D  
 Acq On : 9 Nov 21 12:13  
 Sample : 0.5ug/L VOC STD 11/9/21  
 Misc : IS&S 8/15/21

Vial: 3  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 10 9:44 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 09:43:41 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
40) 3-Methylpentane	3.34	57	76	0.12	ppb	# 19
41) Chloroform	5.29	83	1131	0.45	ppb	100
42) Bromochloromethane	5.14	49	184	0.21	ppb	# 43
44) 1,1,1-TCA	5.49	97	825	0.76	ppb	# 65
45) Cyclohexane	5.56	56	699	0.39	ppb	# 55
46) 1,1-Dichloropropene	5.73	75	832	0.47	ppb	# 75
47) 2,2,4-Trimethylpentane	6.13	57	1433	0.36	ppb	# 65
49) Carbon Tetrachloride	5.72	117	1100	0.48	ppb	# 62
50) Tert Amyl Methyl Ether	6.19	73	1666	0.46	ppb	# 90
52) 1,2-DCA	6.01	62	1065	0.56	ppb	# 73
53) Benzene	5.98	78	2519	0.47	ppb	# 91
54) TCE	6.79	130	467	0.45	ppb	# 70
55) 2-Pentanone	7.06	43	19034	21.96	ppb	# 99
56) 1,2-Dichloropropane	7.05	63	494	0.36	ppb	# 84
57) Bromodichloromethane	7.41	83	1033	0.53	ppb	# 93
58) Methyl Cyclohexane	7.02	83	1207	0.51	ppb	# 63
59) Dibromomethane	7.19	174	1043	0.67	ppb	# 82
60) MIBK (methyl isobutyl ket	8.13	43	9087	7.60	ppb	# 96
61) 1-Bromo-2-chloroethane	7.74	63	474	0.51	ppb	# 48
63) Cis-1,3-Dichloropropene	7.93	75	1046	0.48	ppb	# 87
64) Toluene	8.29	91	3479	0.51	ppb	# 79
65) Trans-1,3-Dichloropropene	8.56	75	978	0.48	ppb	# 52
66) 1,1,2-TCA	8.76	97	663	0.46	ppb	# 84
67) 2-Hexanone	9.06	43	6351	7.70	ppb	# 87
70) 1,2-EDB	9.28	107	665	0.41	ppb	# 81
71) Tetrachloroethene	8.91	166	1574	0.56	ppb	# 82
72) 1-Chlorohexane	9.85	91	1446	0.61	ppb	# 86
73) 1,1,1,2-Tetrachloroethane	9.94	131	1003	0.51	ppb	# 90
74) m&p-Xylene	10.11	91	5770	1.27	ppb	# 92
75) o-Xylene	10.54	91	3153	0.49	ppb	# 99
76) Styrene	10.57	104	2255	0.45	ppb	# 93
78) 1,3-Dichloropropane	8.93	76	914	0.40	ppb	# 82
79) Dibromochloromethane	9.17	129	991	0.49	ppb	# 74
80) Chlorobenzene	9.85	112	2618	0.49	ppb	# 98
81) Ethylbenzene	9.98	91	4006	0.50	ppb	# 94
82) Bromoform	10.75	173	820	0.47	ppb	# 77
84) Isopropylbenzene	10.95	105	3865	0.44	ppb	# 98
85) 1,1,2,2-Tetrachloroethane	11.27	83	821	0.40	ppb	# 88
86) 1,2,3-Trichloropropane	11.31	110	254	0.35	ppb	# 33
88) Bromobenzene	11.27	156	1574	0.54	ppb	# 89
89) n-Propylbenzene	11.40	91	4533	0.46	ppb	# 96
90) 4-Ethyltoluene	11.52	105	4219	0.49	ppb	# 91

(#) = qualifier out of range (m) = manual integration  
 1109T15.D T1109W.M Thu Nov 11 11:38:41 2021

Data File : M:\THOR\DATA\211109\1109T15.D  
 Acq On : 9 Nov 21 12:13  
 Sample : 0.5ug/L VOC STD 11/9/21  
 Misc : IS&S 8/15/21

Vial: 3  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 10 9:44 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 09:43:41 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
91) 2-Chlorotoluene	11.49	91	2668	0.40	ppb	94
92) 1,3,5-Trimethylbenzene	11.60	105	3580	0.48	ppb	95
93) 4-Chlorotoluene	11.60	91	2915	0.43	ppb	99
94) Tert-Butylbenzene	11.95	119	3178	0.40	ppb	95
95) 1,2,4-Trimethylbenzene	12.01	105	3658	0.50	ppb	94
96) Sec-Butylbenzene	12.19	105	4111	0.43	ppb	99
97) p-Isopropyltoluene	12.35	119	3900	0.46	ppb	95
98) Benzyl Chloride	12.54	91	1512	0.42	ppb #	87
99) 1,3-DCB	12.40	146	2872	0.55	ppb	92
100) 1,4-DCB	12.40	146	2872	0.54	ppb	92
101) n-Butylbenzene	12.80	91	2611	0.39	ppb	95
102) 1,2-DCB	12.81	146	2478	0.52	ppb #	85
103) Hexachloroethane	13.09	201	498	0.28	ppb #	83
104) 1,2-Dibromo-3-chloropropan	13.64	157	108	0.21	ppb #	66
105) 1,2,4-Trichlorobenzene	14.57	180	1793	0.53	ppb #	60
106) Hexachlorobutadiene	14.76	225	1452	0.71	ppb	97
107) Naphthalene	14.83	128	1367	0.45	ppb	97
108) 1,2,3-Trichlorobenzene	15.11	180	1546	0.49	ppb	80

Quantitation Report


Data File : M:\THOR\DATA\211109\1109T15.D  
Acq On : 9 Nov 21 12:13  
Sample : 0.5ug/L VOC STD 11/9/21  
Misc : IS&S 8/15/21

Vial: 3  
Operator:  
Inst : Thor  
Multiplr: 1.00

Quant Time: Nov 10 9:44 2021

Quant Results File: T1109W.RES

Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Wed Nov 10 10:21:13 2021  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data File : M:\THOR\DATA\211109\1109T16.D  
 Acq On : 9 Nov 21 12:38  
 Sample : 1ug/L VOC STD 11/9/21  
 Misc : IS&S 8/15/21

Vial: 4  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 10 9:44 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 09:43:41 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.35	96	315410	25.00	ppb	0.00
68) Chlorobenzene-D5 (IS)	9.81	117	306467	25.00	ppb	0.00
83) 1,4-Dichlorobenzene-D (IS)	12.37	152	215832	25.00	ppb	0.00
System Monitoring Compounds						
43) Dibromofluoromethane(S)	5.49	111	33848	10.22	ppb	0.00
Spiked Amount	25.000		Recovery	=	40.884%	
48) 1,2-DCA-D4(S)	5.91	65	36872	11.21	ppb	0.00
Spiked Amount	25.000		Recovery	=	44.836%	
69) Toluene-D8(S)	8.22	98	115490	9.25	ppb	0.00
Spiked Amount	25.000		Recovery	=	37.016%	
77) 4-Bromofluorobenzene(S)	11.11	95	45103	9.35	ppb	0.00
Spiked Amount	25.000		Recovery	=	37.388%	
Target Compounds						
4) Freon 114	1.20	85	527	-0.15	ppb	94
5) Chloromethane	1.28	50	505	1.15	ppb	93
6) Vinyl chloride	1.33	62	772	0.69	ppb	89
7) Butane	1.59	43	20	19.09	ppb	# 100
9) Bromomethane	1.59	96	767	0.99	ppb	99
10) Chloroethane	1.68	64	574	1.01	ppb	# 48
11) Dichlorofluoromethane	1.87	67	2063	1.05	ppb	91
12) Trichlorofluoromethane	1.91	101	2934	1.17	ppb	87
16) Acrolein	2.31	56	8047	50.81	ppb	84
17) Acetone	2.48	43	5627	17.68	ppb	# 67
18) Freon-113	2.43	101	660	1.01	ppb	# 77
19) 1,1-DCE	2.41	61	1792	0.98	ppb	94
21) Acetonitrile	2.80	40	708	38.54	ppb	84
22) t-Butanol	3.17	59	1894	52.47	ppb	# 89
23) Methyl Acetate	2.90	43	295	0.40	ppb	# 40
24) Iodomethane	2.55	142	781	0.86	ppb	# 85
26) Methylene chloride	2.96	49	1099	0.62	ppb	88
27) Carbon disulfide	2.62	76	1408	0.92	ppb	98
28) Methyl t-butyl ether (MtBE)	3.34	73	3384	1.01	ppb	93
29) Trans-1,2-DCE	3.32	61	1208	0.77	ppb	# 82
31) Diisopropyl Ether	4.13	45	2286	0.76	ppb	88
33) 1,1-DCA	3.93	63	2040	1.01	ppb	# 82
34) Vinyl Acetate	4.12	43	816	0.92	ppb	# 84
35) Ethyl tert Butyl Ether	4.68	59	2559	0.78	ppb	89
36) MEK (2-Butanone)	4.88	43	7420	16.48	ppb	95
37) Cis-1,2-DCE	4.82	61	1507	0.78	ppb	# 78
38) 2,2-Dichloropropane	4.80	77	2266	1.07	ppb	# 80

(#) = qualifier out of range (m) = manual integration  
 1109T16.D T1109W.M Thu Nov 11 11:38:42 2021



Quantitation Report (Not Reviewed)

Data File : M:\THOR\DATA\211109\1109T16.D  
 Acq On : 9 Nov 21 12:38  
 Sample : 1ug/L VOC STD 11/9/21  
 Misc : IS&S 8/15/21

Vial: 4  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 10 9:44 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 09:43:41 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
39) 2-Methylpentane	3.17	43	963	3.70	ppb	# 87
40) 3-Methylpentane	3.34	57	578	0.88	ppb	# 62
41) Chloroform	5.29	83	2371	0.92	ppb	96
42) Bromochloromethane	5.14	49	702	0.81	ppb	# 77
44) 1,1,1-TCA	5.49	97	1329	1.21	ppb	# 84
45) Cyclohexane	5.56	56	1501	0.83	ppb	# 81
46) 1,1-Dichloropropene	5.72	75	1647	0.92	ppb	# 79
47) 2,2,4-Trimethylpentane	6.13	57	3538	0.87	ppb	94
49) Carbon Tetrachloride	5.70	117	2832	1.22	ppb	96
50) Tert Amyl Methyl Ether	6.19	73	3447	0.94	ppb	94
52) 1,2-DCA	6.02	62	2055	1.07	ppb	# 73
53) Benzene	5.98	78	5099	0.95	ppb	94
54) TCE	6.80	130	1187	1.13	ppb	94
55) 2-Pentanone	7.06	43	38143	43.41	ppb	97
56) 1,2-Dichloropropane	7.05	63	1247	0.90	ppb	# 84
57) Bromodichloromethane	7.40	83	1989	1.00	ppb	94
58) Methyl Cyclohexane	7.01	83	2428	1.01	ppb	95
59) Dibromomethane	7.19	174	2020	1.29	ppb	95
60) MIBK (methyl isobutyl ket	8.12	43	19060	15.72	ppb	93
61) 1-Bromo-2-chloroethane	7.73	63	685	0.72	ppb	# 88
63) Cis-1,3-Dichloropropene	7.92	75	2141	0.96	ppb	# 83
64) Toluene	8.29	91	6354	0.92	ppb	95
65) Trans-1,3-Dichloropropene	8.56	75	1759	0.85	ppb	95
66) 1,1,2-TCA	8.75	97	1536	1.06	ppb	# 71
67) 2-Hexanone	9.06	43	12735	15.23	ppb	99
70) 1,2-EDB	9.29	107	1513	0.91	ppb	# 72
71) Tetrachloroethene	8.90	166	3279	1.14	ppb	93
72) 1-Chlorohexane	9.84	91	3035	1.26	ppb	# 86
73) 1,1,1,2-Tetrachloroethane	9.94	131	2233	1.12	ppb	87
74) m&p-Xylene	10.11	91	12091	2.24	ppb	88
75) o-Xylene	10.54	91	6382	0.98	ppb	98
76) Styrene	10.56	104	4393	0.86	ppb	# 80
78) 1,3-Dichloropropane	8.93	76	2122	0.91	ppb	# 75
79) Dibromochloromethane	9.18	129	2119	1.03	ppb	# 78
80) Chlorobenzene	9.84	112	5172	0.95	ppb	99
81) Ethylbenzene	9.98	91	7839	0.97	ppb	96
82) Bromoform	10.74	173	2358	1.34	ppb	# 89
84) Isopropylbenzene	10.95	105	8227	0.88	ppb	97
85) 1,1,2,2-Tetrachloroethane	11.27	83	1570	0.74	ppb	92
86) 1,2,3-Trichloropropane	11.31	110	984	1.28	ppb	# 80
87) t-1,4-Dichloro-2-Butene	11.34	53	128	0.28	ppb	# 34
88) Bromobenzene	11.26	156	3079	1.01	ppb	91

Data File : M:\THOR\DATA\211109\1109T16.D  
 Acq On : 9 Nov 21 12:38  
 Sample : 1ug/L VOC STD 11/9/21  
 Misc : IS&S 8/15/21

Vial: 4  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 10 9:44 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 09:43:41 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
89) n-Propylbenzene	11.40	91	8988	0.87	ppb	91
90) 4-Ethyltoluene	11.53	105	7931	0.88	ppb	92
91) 2-Chlorotoluene	11.48	91	6528	0.93	ppb	98
92) 1,3,5-Trimethylbenzene	11.60	105	7582	0.97	ppb	93
93) 4-Chlorotoluene	11.61	91	6467	0.91	ppb	96
94) Tert-Butylbenzene	11.95	119	8066	0.96	ppb	99
95) 1,2,4-Trimethylbenzene	12.00	105	6924	0.90	ppb	95
96) Sec-Butylbenzene	12.19	105	8380	0.84	ppb	90
97) p-Isopropyltoluene	12.36	119	8085	0.90	ppb	99
98) Benzyl Chloride	12.54	91	2939	0.78	ppb	95
99) 1,3-DCB	12.30	146	5213	0.95	ppb	88
100) 1,4-DCB	12.39	146	5880	1.05	ppb	92
101) n-Butylbenzene	12.80	91	5729	0.83	ppb	97
102) 1,2-DCB	12.80	146	4941	0.98	ppb	92
103) Hexachloroethane	13.08	201	1806	0.95	ppb	# 84
104) 1,2-Dibromo-3-chloropropan	13.65	157	412	0.75	ppb	# 76
105) 1,2,4-Trichlorobenzene	14.56	180	3464	0.98	ppb	100
106) Hexachlorobutadiene	14.76	225	2378	1.10	ppb	96
107) Naphthalene	14.83	128	2604	0.82	ppb	99
108) 1,2,3-Trichlorobenzene	15.10	180	3314	1.00	ppb	# 75

Quantitation Report


Data File : M:\THOR\DATA\211109\1109T16.D  
Acq On : 9 Nov 21 12:38  
Sample : 1ug/L VOC STD 11/9/21  
Misc : IS&S 8/15/21

Vial: 4  
Operator:  
Inst : Thor  
Multiplr: 1.00

Quant Time: Nov 10 9:44 2021

Quant Results File: T1109W.RES

Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Wed Nov 10 10:21:13 2021  
Response via : Initial Calibration



Data File : M:\THOR\DATA\211109\1109T17.D  
 Acq On : 9 Nov 21 13:03  
 Sample : 2ug/L VOC STD 11/9/21  
 Misc : IS&S 8/15/21

Vial: 5  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 10 9:44 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 09:43:41 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.35	96	310022	25.00	ppb	0.00
68) Chlorobenzene-D5 (IS)	9.81	117	303468	25.00	ppb	0.00
83) 1,4-Dichlorobenzene-D (IS)	12.37	152	213648	25.00	ppb	0.00
System Monitoring Compounds						
43) Dibromofluoromethane(S)	5.49	111	33616	10.33	ppb	0.00
Spiked Amount	25.000		Recovery	=	41.308%	
48) 1,2-DCA-D4(S)	5.91	65	35345	10.93	ppb	0.00
Spiked Amount	25.000		Recovery	=	43.728%	
69) Toluene-D8(S)	8.22	98	115701	9.36	ppb	0.00
Spiked Amount	25.000		Recovery	=	37.448%	
77) 4-Bromofluorobenzene(S)	11.11	95	45552	9.53	ppb	0.00
Spiked Amount	25.000		Recovery	=	38.136%	
Target Compounds						Qvalue
3) Dichlorodifluoromethane	1.10	85	2244	1.15	ppb	96
4) Freon 114	1.20	85	1508	1.24	ppb	# 72
5) Chloromethane	1.28	50	711	1.64	ppb	96
6) Vinyl chloride	1.32	62	1627	1.49	ppb	# 84
9) Bromomethane	1.59	96	1747	2.30	ppb	98
10) Chloroethane	1.68	64	1168	2.10	ppb	95
11) Dichlorofluoromethane	1.87	67	3848	1.99	ppb	# 79
12) Trichlorofluoromethane	1.91	101	6618	2.68	ppb	97
16) Acrolein	2.31	56	11593	74.48	ppb	92
17) Acetone	2.48	43	8797	28.12	ppb	91
18) Freon-113	2.43	101	1637	2.55	ppb	# 88
19) 1,1-DCE	2.41	61	3825	2.20	ppb	99
21) Acetonitrile	2.78	40	1101	61.88	ppb	# 93
22) t-Butanol	3.16	59	3200	90.19	ppb	# 85
23) Methyl Acetate	2.88	43	968	1.34	ppb	# 40
24) Iodomethane	2.55	142	1842	2.91	ppb	91
25) Acrylonitrile	3.37	52	20	2.48	ppb	# 6
26) Methylene chloride	2.96	49	2061	1.39	ppb	92
27) Carbon disulfide	2.61	76	3616	2.40	ppb	96
28) Methyl t-butyl ether (MtBE)	3.34	73	6482	1.97	ppb	92
29) Trans-1,2-DCE	3.32	61	2736	1.77	ppb	# 84
31) Diisopropyl Ether	4.13	45	4271	1.45	ppb	99
33) 1,1-DCA	3.92	63	3424	1.72	ppb	99
34) Vinyl Acetate	4.12	43	1998	1.41	ppb	# 84
35) Ethyl tert Butyl Ether	4.68	59	5711	1.77	ppb	# 75
36) MEK (2-Butanone)	4.88	43	10986	24.83	ppb	98
37) Cis-1,2-DCE	4.82	61	3472	1.84	ppb	# 81

(#) = qualifier out of range (m) = manual integration  
 1109T17.D T1109W.M Thu Nov 11 11:38:45 2021

Data File : M:\THOR\DATA\211109\1109T17.D  
 Acq On : 9 Nov 21 13:03  
 Sample : 2ug/L VOC STD 11/9/21  
 Misc : IS&S 8/15/21

Vial: 5  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 10 9:44 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 09:43:41 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
38) 2,2-Dichloropropane	4.80	77	4679	2.25	ppb	96
39) 2-Methylpentane	3.16	43	1783	6.96	ppb #	63
40) 3-Methylpentane	3.35	57	1144	1.77	ppb #	80
41) Chloroform	5.29	83	5470	2.16	ppb	95
42) Bromochloromethane	5.13	49	1407	1.65	ppb #	70
44) 1,1,1-TCA	5.48	97	2335	2.16	ppb #	86
45) Cyclohexane	5.56	56	3318	1.86	ppb #	70
46) 1,1-Dichloropropene	5.73	75	3668	2.09	ppb	99
47) 2,2,4-Trimethylpentane	6.13	57	7398	1.85	ppb	100
49) Carbon Tetrachloride	5.71	117	4927	2.17	ppb	96
50) Tert Amyl Methyl Ether	6.18	73	6819	1.89	ppb #	90
51) Methylcyclopentane	4.67	56	112	0.81	ppb	100
52) 1,2-DCA	6.01	62	3963	2.10	ppb #	94
53) Benzene	5.97	78	9763	1.84	ppb	96
54) TCE	6.80	130	2234	2.16	ppb	91
55) 2-Pentanone	7.06	43	56409	65.31	ppb	97
56) 1,2-Dichloropropane	7.05	63	2230	1.64	ppb #	81
57) Bromodichloromethane	7.40	83	4343	2.22	ppb	92
58) Methyl Cyclohexane	7.01	83	4515	1.91	ppb	98
59) Dibromomethane	7.19	174	3706	2.40	ppb #	89
60) MIBK (methyl isobutyl ket	8.12	43	29374	24.65	ppb	96
61) 1-Bromo-2-chloroethane	7.73	63	1599	1.71	ppb	90
62) 2-Chloroethyl vinyl ether	7.81	44	43	104.40	ppb	100
63) Cis-1,3-Dichloropropene	7.92	75	4347	1.98	ppb	93
64) Toluene	8.30	91	13414	1.99	ppb	97
65) Trans-1,3-Dichloropropene	8.56	75	4137	2.04	ppb	97
66) 1,1,2-TCA	8.76	97	2869	2.02	ppb	86
67) 2-Hexanone	9.06	43	20853	25.38	ppb #	89
70) 1,2-EDB	9.29	107	3228	1.97	ppb	97
71) Tetrachloroethene	8.90	166	6744	2.38	ppb	98
72) 1-Chlorohexane	9.85	91	4440	1.87	ppb #	87
73) 1,1,1,2-Tetrachloroethane	9.94	131	4415	2.23	ppb #	92
74) m&p-Xylene	10.11	91	23618	4.07	ppb	91
75) o-Xylene	10.54	91	12068	1.88	ppb	91
76) Styrene	10.56	104	9229	1.83	ppb	97
78) 1,3-Dichloropropane	8.94	76	4023	1.74	ppb	99
79) Dibromochloromethane	9.18	129	4184	2.06	ppb	84
80) Chlorobenzene	9.85	112	10771	2.01	ppb	97
81) Ethylbenzene	9.98	91	15670	1.95	ppb	97
82) Bromoform	10.74	173	4271	2.45	ppb	89
84) Isopropylbenzene	10.95	105	15998	1.73	ppb	91
85) 1,1,2,2-Tetrachloroethane	11.27	83	3070	1.45	ppb #	92

(#) = qualifier out of range (m) = manual integration  
 1109T17.D T1109W.M Thu Nov 11 11:38:45 2021

Data File : M:\THOR\DATA\211109\1109T17.D  
 Acq On : 9 Nov 21 13:03  
 Sample : 2ug/L VOC STD 11/9/21  
 Misc : IS&S 8/15/21

Vial: 5  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 10 9:44 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 09:43:41 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
86) 1,2,3-Trichloropropane	11.31	110	1546	2.03	ppb	# 74
87) t-1,4-Dichloro-2-Butene	11.34	53	824	1.84	ppb	# 77
88) Bromobenzene	11.26	156	6353	2.10	ppb	90
89) n-Propylbenzene	11.40	91	18612	1.82	ppb	95
90) 4-Ethyltoluene	11.53	105	16268	1.83	ppb	97
91) 2-Chlorotoluene	11.49	91	12523	1.80	ppb	98
92) 1,3,5-Trimethylbenzene	11.60	105	14270	1.84	ppb	97
93) 4-Chlorotoluene	11.60	91	12623	1.79	ppb	99
94) Tert-Butylbenzene	11.95	119	16197	1.95	ppb	92
95) 1,2,4-Trimethylbenzene	12.00	105	13983	1.83	ppb	88
96) Sec-Butylbenzene	12.19	105	18057	1.84	ppb	99
97) p-Isopropyltoluene	12.36	119	16774	1.89	ppb	100
98) Benzyl Chloride	12.55	91	6119	1.65	ppb	99
99) 1,3-DCB	12.30	146	10852	1.99	ppb	99
100) 1,4-DCB	12.40	146	11112	2.01	ppb	# 92
101) n-Butylbenzene	12.80	91	12233	1.78	ppb	99
102) 1,2-DCB	12.80	146	9825	1.97	ppb	95
103) Hexachloroethane	13.09	201	4072	2.17	ppb	93
104) 1,2-Dibromo-3-chloropropan	13.64	157	1069	1.97	ppb	# 79
105) 1,2,4-Trichlorobenzene	14.56	180	7242	2.08	ppb	95
106) Hexachlorobutadiene	14.76	225	5205	2.43	ppb	95
107) Naphthalene	14.83	128	5868	1.87	ppb	99
108) 1,2,3-Trichlorobenzene	15.09	180	7125	2.18	ppb	95

Quantitation Report


Data File : M:\THOR\DATA\211109\1109T17.D  
Acq On : 9 Nov 21 13:03  
Sample : 2ug/L VOC STD 11/9/21  
Misc : IS&S 8/15/21

Vial: 5  
Operator:  
Inst : Thor  
Multiplr: 1.00

Quant Time: Nov 10 9:44 2021

Quant Results File: T1109W.RES

Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Wed Nov 10 10:21:13 2021  
Response via : Initial Calibration



Data File : M:\THOR\DATA\211109\1109T18.D  
 Acq On : 9 Nov 21 13:28  
 Sample : 5ug/L VOC STD 11/9/21  
 Misc : IS&S 8/15/21

Vial: 6  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 10 9:44 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 09:43:41 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.35	96	308169	25.00	ppb	0.00
68) Chlorobenzene-D5 (IS)	9.81	117	300381	25.00	ppb	0.00
83) 1,4-Dichlorobenzene-D (IS)	12.37	152	211820	25.00	ppb	0.00
System Monitoring Compounds						
43) Dibromofluoromethane(S)	5.49	111	92209	28.50	ppb	0.00
Spiked Amount	25.000		Recovery	=	113.996%	
48) 1,2-DCA-D4(S)	5.91	65	97737	30.41	ppb	0.00
Spiked Amount	25.000		Recovery	=	121.644%	
69) Toluene-D8(S)	8.22	98	310849	25.41	ppb	0.00
Spiked Amount	25.000		Recovery	=	101.648%	
77) 4-Bromofluorobenzene(S)	11.11	95	123771	26.17	ppb	0.00
Spiked Amount	25.000		Recovery	=	104.684%	
Target Compounds						Qvalue
3) Dichlorodifluoromethane	1.09	85	4778	4.99	ppb	100
4) Freon 114	1.20	85	3932	4.68	ppb	96
5) Chloromethane	1.28	50	1502	3.49	ppb	99
6) Vinyl chloride	1.33	62	3867	3.56	ppb	99
7) Butane	1.55	43	21	20.52	ppb	# 100
9) Bromomethane	1.60	96	3454	4.57	ppb	98
10) Chloroethane	1.68	64	2520	4.55	ppb	95
11) Dichlorofluoromethane	1.86	67	8144	4.24	ppb	100
12) Trichlorofluoromethane	1.91	101	13560	5.52	ppb	98
16) Acrolein	2.31	56	15309	98.94	ppb	97
17) Acetone	2.48	43	12119	38.98	ppb	# 89
18) Freon-113	2.43	101	2677	4.20	ppb	98
19) 1,1-DCE	2.41	61	7155	4.20	ppb	# 91
21) Acetonitrile	2.78	40	1591	92.54	ppb	89
22) t-Butanol	3.17	59	3923	111.24	ppb	93
23) Methyl Acetate	2.88	43	1859	2.58	ppb	98
24) Iodomethane	2.55	142	3220	5.58	ppb	97
25) Acrylonitrile	3.32	52	497	3.82	ppb	# 70
26) Methylene chloride	2.96	49	4846	3.58	ppb	90
27) Carbon disulfide	2.61	76	6278	4.19	ppb	97
28) Methyl t-butyl ether (MtBE)	3.34	73	13984	4.28	ppb	92
29) Trans-1,2-DCE	3.32	61	6218	4.04	ppb	95
31) Diisopropyl Ether	4.12	45	9673	3.30	ppb	96
33) 1,1-DCA	3.93	63	7417	3.75	ppb	# 92
34) Vinyl Acetate	4.12	43	6006	3.05	ppb	# 84
35) Ethyl tert Butyl Ether	4.68	59	12816	4.00	ppb	# 80
36) MEK (2-Butanone)	4.87	43	14744	33.52	ppb	92

(#) = qualifier out of range (m) = manual integration  
 1109T18.D T1109W.M Thu Nov 11 11:38:47 2021



Quantitation Report (Not Reviewed)

Data File : M:\THOR\DATA\211109\1109T18.D  
 Acq On : 9 Nov 21 13:28  
 Sample : 5ug/L VOC STD 11/9/21  
 Misc : IS&S 8/15/21

Vial: 6  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 10 9:44 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 09:43:41 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
37) Cis-1,2-DCE	4.81	61	7349	3.91	ppb	91
38) 2,2-Dichloropropane	4.79	77	9517	4.60	ppb	98
39) 2-Methylpentane	3.15	43	2352	9.24	ppb #	57
40) 3-Methylpentane	3.34	57	2318	3.61	ppb	86
41) Chloroform	5.29	83	11123	4.42	ppb	99
42) Bromochloromethane	5.13	49	3157	3.72	ppb	84
44) 1,1,1-TCA	5.49	97	5308	4.93	ppb	100
45) Cyclohexane	5.55	56	6094	3.43	ppb #	73
46) 1,1-Dichloropropene	5.72	75	7176	4.11	ppb	96
47) 2,2,4-Trimethylpentane	6.13	57	14237	3.58	ppb	92
49) Carbon Tetrachloride	5.71	117	11911	5.27	ppb	96
50) Tert Amyl Methyl Ether	6.18	73	13854	3.86	ppb	98
51) Methylcyclopentane	4.67	56	475	3.44	ppb	100
52) 1,2-DCA	6.01	62	9063	4.84	ppb #	94
53) Benzene	5.97	78	20780	3.94	ppb	99
54) TCE	6.80	130	4686	4.57	ppb	95
55) 2-Pentanone	7.05	43	77349	90.09	ppb	98
56) 1,2-Dichloropropane	7.05	63	4492	3.32	ppb #	92
57) Bromodichloromethane	7.40	83	8427	4.34	ppb	95
58) Methyl Cyclohexane	7.01	83	8910	3.80	ppb	97
59) Dibromomethane	7.18	174	8113	5.29	ppb #	87
60) MIBK (methyl isobutyl ket	8.12	43	40580	34.25	ppb	99
61) 1-Bromo-2-chloroethane	7.73	63	3170	3.42	ppb	94
63) Cis-1,3-Dichloropropene	7.93	75	8028	3.68	ppb	88
64) Toluene	8.29	91	26958	4.01	ppb	100
65) Trans-1,3-Dichloropropene	8.56	75	8356	4.14	ppb	91
66) 1,1,2-TCA	8.75	97	5983	4.23	ppb	96
67) 2-Hexanone	9.06	43	28299	34.65	ppb	97
70) 1,2-EDB	9.29	107	6970	4.29	ppb #	96
71) Tetrachloroethene	8.90	166	14156	5.04	ppb	91
72) 1-Chlorohexane	9.85	91	9275	3.94	ppb	91
73) 1,1,1,2-Tetrachloroethane	9.94	131	9317	4.75	ppb	93
74) m&p-Xylene	10.11	91	53654	8.89	ppb	98
75) o-Xylene	10.54	91	26271	4.13	ppb	94
76) Styrene	10.56	104	19719	3.96	ppb	95
78) 1,3-Dichloropropane	8.94	76	9066	3.97	ppb	89
79) Dibromochloromethane	9.18	129	9180	4.56	ppb	98
80) Chlorobenzene	9.85	112	22574	4.25	ppb	97
81) Ethylbenzene	9.98	91	32529	4.09	ppb	94
82) Bromoform	10.75	173	7943	4.60	ppb	94
84) Isopropylbenzene	10.95	105	34287	3.75	ppb	93
85) 1,1,2,2-Tetrachloroethane	11.27	83	7389	3.53	ppb	96

(#) = qualifier out of range (m) = manual integration  
 1109T18.D T1109W.M Thu Nov 11 11:38:47 2021

Data File : M:\THOR\DATA\211109\1109T18.D  
 Acq On : 9 Nov 21 13:28  
 Sample : 5ug/L VOC STD 11/9/21  
 Misc : IS&S 8/15/21

Vial: 6  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 10 9:44 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 09:43:41 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
86) 1,2,3-Trichloropropane	11.31	110	2848	3.77	ppb	# 70
87) t-1,4-Dichloro-2-Butene	11.34	53	1462	3.30	ppb	# 64
88) Bromobenzene	11.27	156	13197	4.40	ppb	95
89) n-Propylbenzene	11.40	91	37964	3.75	ppb	98
90) 4-Ethyltoluene	11.53	105	34689	3.94	ppb	96
91) 2-Chlorotoluene	11.48	91	26714	3.88	ppb	94
92) 1,3,5-Trimethylbenzene	11.60	105	31368	4.08	ppb	100
93) 4-Chlorotoluene	11.60	91	27612	3.94	ppb	97
94) Tert-Butylbenzene	11.95	119	33365	4.06	ppb	95
95) 1,2,4-Trimethylbenzene	12.00	105	29028	3.83	ppb	89
96) Sec-Butylbenzene	12.19	105	37095	3.81	ppb	93
97) p-Isopropyltoluene	12.35	119	36564	4.15	ppb	96
98) Benzyl Chloride	12.54	91	14604	3.97	ppb	97
99) 1,3-DCB	12.30	146	22943	4.24	ppb	96
100) 1,4-DCB	12.40	146	24395	4.44	ppb	# 87
101) n-Butylbenzene	12.80	91	25897	3.80	ppb	98
102) 1,2-DCB	12.80	146	20077	4.05	ppb	97
103) Hexachloroethane	13.08	201	9523	5.13	ppb	96
104) 1,2-Dibromo-3-chloropropan	13.64	157	2484	4.62	ppb	93
105) 1,2,4-Trichlorobenzene	14.57	180	15167	4.38	ppb	89
106) Hexachlorobutadiene	14.76	225	10383	4.89	ppb	96
107) Naphthalene	14.83	128	11602	3.74	ppb	98
108) 1,2,3-Trichlorobenzene	15.10	180	13872	4.28	ppb	87



Data File : M:\THOR\DATA\211109\1109T19.D  
 Acq On : 9 Nov 21 13:52  
 Sample : 10ug/L VOC STD 11/9/21  
 Misc : IS&S 8/15/21

Vial: 7  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 10 9:44 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 09:43:41 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.35	96	316124	25.00	ppb	0.00
68) Chlorobenzene-D5 (IS)	9.81	117	306509	25.00	ppb	0.00
83) 1,4-Dichlorobenzene-D (IS)	12.37	152	216025	25.00	ppb	0.00

System Monitoring Compounds

43) Dibromofluoromethane(S)	5.49	111	93942	28.30	ppb	0.00
Spiked Amount	25.000		Recovery	=	113.216%	
48) 1,2-DCA-D4(S)	5.91	65	98718	29.94	ppb	0.00
Spiked Amount	25.000		Recovery	=	119.772%	
69) Toluene-D8(S)	8.22	98	315563	25.28	ppb	0.00
Spiked Amount	25.000		Recovery	=	101.128%	
77) 4-Bromofluorobenzene(S)	11.11	95	127947	26.51	ppb	0.00
Spiked Amount	25.000		Recovery	=	106.052%	

Target Compounds

	R.T.	QIon	Response	Conc	Units	Qvalue
3) Dichlorodifluoromethane	1.10	85	11150	14.17	ppb	100
4) Freon 114	1.20	85	9438	12.11	ppb	100
5) Chloromethane	1.28	50	3549	8.05	ppb	100
6) Vinyl chloride	1.33	62	8927	8.00	ppb	100
7) Butane	1.60	43	21	20.00	ppb	# 100
9) Bromomethane	1.59	96	7109	9.16	ppb	100
10) Chloroethane	1.68	64	5308	9.34	ppb	100
11) Dichlorofluoromethane	1.86	67	19709	9.99	ppb	100
12) Trichlorofluoromethane	1.91	101	32001	12.70	ppb	100
16) Acrolein	2.31	56	20651	130.11	ppb	100
17) Acetone	2.48	43	16030	50.26	ppb	100
18) Freon-113	2.43	101	6773	10.35	ppb	100
19) 1,1-DCE	2.41	61	19198	11.10	ppb	100
21) Acetonitrile	2.79	40	1799	103.12	ppb	100
22) t-Butanol	3.16	59	5029	139.01	ppb	100
23) Methyl Acetate	2.87	43	5736	7.77	ppb	100
24) Iodomethane	2.55	142	7471	13.39	ppb	100
25) Acrylonitrile	3.30	52	1855	7.49	ppb	100
26) Methylene chloride	2.96	49	12589	9.42	ppb	100
27) Carbon disulfide	2.61	76	15247	9.91	ppb	100
28) Methyl t-butyl ether (MtBE)	3.33	73	34460	10.28	ppb	100
29) Trans-1,2-DCE	3.31	61	15568	9.85	ppb	100
31) Diisopropyl Ether	4.11	45	24119	8.01	ppb	100
33) 1,1-DCA	3.92	63	19095	9.41	ppb	100
34) Vinyl Acetate	4.11	43	17813	7.70	ppb	100
35) Ethyl tert Butyl Ether	4.68	59	30949	9.41	ppb	100
36) MEK (2-Butanone)	4.87	43	19811	43.91	ppb	100

Data File : M:\THOR\DATA\211109\1109T19.D  
 Acq On : 9 Nov 21 13:52  
 Sample : 10ug/L VOC STD 11/9/21  
 Misc : IS&S 8/15/21

Vial: 7  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 10 9:44 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 09:43:41 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
37) Cis-1,2-DCE	4.81	61	18459	9.58	ppb	100
38) 2,2-Dichloropropane	4.79	77	22877	10.79	ppb	100
39) 2-Methylpentane	3.16	43	2611	10.00	ppb	100
40) 3-Methylpentane	3.34	57	6579	10.00	ppb	100
41) Chloroform	5.28	83	29401	11.39	ppb	100
42) Bromochloromethane	5.13	49	7824	8.98	ppb	100
44) 1,1,1-TCA	5.49	97	12882	11.67	ppb	100
45) Cyclohexane	5.55	56	16975	9.32	ppb	100
46) 1,1-Dichloropropene	5.72	75	17988	10.04	ppb	100
47) 2,2,4-Trimethylpentane	6.13	57	36718	9.00	ppb	100
49) Carbon Tetrachloride	5.71	117	28776	12.41	ppb	100
50) Tert Amyl Methyl Ether	6.18	73	35489	9.64	ppb	100
51) Methylcyclopentane	4.67	56	1415	10.00	ppb	100
52) 1,2-DCA	6.01	62	20716	10.79	ppb	100
53) Benzene	5.97	78	50647	9.37	ppb	100
54) TCE	6.80	130	11441	10.87	ppb	100
55) 2-Pentanone	7.05	43	98257	111.56	ppb	100
56) 1,2-Dichloropropane	7.05	63	12219	8.80	ppb	100
57) Bromodichloromethane	7.40	83	20664	10.37	ppb	100
58) Methyl Cyclohexane	7.02	83	24292	10.09	ppb	100
59) Dibromomethane	7.19	174	20052	12.74	ppb	100
60) MIBK (methyl isobutyl ket	8.12	43	52383	43.10	ppb	100
61) 1-Bromo-2-chloroethane	7.73	63	8386	8.81	ppb	100
62) 2-Chloroethyl vinyl ether	7.81	44	21	50.00	ppb	100
63) Cis-1,3-Dichloropropene	7.92	75	21928	9.81	ppb	100
64) Toluene	8.29	91	68654	9.97	ppb	100
65) Trans-1,3-Dichloropropene	8.56	75	20578	9.93	ppb	100
66) 1,1,2-TCA	8.75	97	13994	9.65	ppb	100
67) 2-Hexanone	9.06	43	37067	44.24	ppb	100
70) 1,2-EDB	9.29	107	17497	10.55	ppb	100
71) Tetrachloroethene	8.90	166	35125	12.25	ppb	100
72) 1-Chlorohexane	9.85	91	22814	9.50	ppb	100
73) 1,1,1,2-Tetrachloroethane	9.94	131	23312	11.65	ppb	100
74) m&p-Xylene	10.11	91	132348	20.98	ppb	100
75) o-Xylene	10.54	91	67348	10.36	ppb	100
76) Styrene	10.56	104	52107	10.25	ppb	100
78) 1,3-Dichloropropane	8.93	76	21677	9.30	ppb	100
79) Dibromochloromethane	9.18	129	22328	10.88	ppb	100
80) Chlorobenzene	9.85	112	55580	10.26	ppb	100
81) Ethylbenzene	9.98	91	81707	10.07	ppb	100
82) Bromoform	10.74	173	22392	12.71	ppb	100
84) Isopropylbenzene	10.95	105	89934	9.64	ppb	100

(#) = qualifier out of range (m) = manual integration  
 1109T19.D T1109W.M Thu Nov 10 09:49:13 2021

Quantitation Report (Not Reviewed)

Data File : M:\THOR\DATA\211109\1109T19.D  
 Acq On : 9 Nov 21 13:52  
 Sample : 10ug/L VOC STD 11/9/21  
 Misc : IS&S 8/15/21

Vial: 7  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 10 9:44 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 09:43:41 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
85) 1,1,2,2-Tetrachloroethane	11.27	83	18330	8.57	ppb	100
86) 1,2,3-Trichloropropane	11.31	110	7993	10.38	ppb	100
87) t-1,4-Dichloro-2-Butene	11.34	53	4721	10.44	ppb	100
88) Bromobenzene	11.26	156	32261	10.54	ppb	100
89) n-Propylbenzene	11.40	91	96209	9.31	ppb	100
90) 4-Ethyltoluene	11.53	105	90312	10.05	ppb	100
91) 2-Chlorotoluene	11.48	91	66926	9.52	ppb	100
92) 1,3,5-Trimethylbenzene	11.60	105	78190	9.98	ppb	100
93) 4-Chlorotoluene	11.60	91	67847	9.50	ppb	100
94) Tert-Butylbenzene	11.95	119	83541	9.96	ppb	100
95) 1,2,4-Trimethylbenzene	12.00	105	77484	10.02	ppb	100
96) Sec-Butylbenzene	12.19	105	96630	9.73	ppb	100
97) p-Isopropyltoluene	12.35	119	92164	10.25	ppb	100
98) Benzyl Chloride	12.55	91	34071	9.08	ppb	100
99) 1,3-DCB	12.30	146	56946	10.32	ppb	100
100) 1,4-DCB	12.40	146	57634	10.29	ppb	100
101) n-Butylbenzene	12.80	91	66078	9.51	ppb	100
102) 1,2-DCB	12.80	146	53596	10.61	ppb	100
103) Hexachloroethane	13.09	201	22066	11.65	ppb	100
104) 1,2-Dibromo-3-chloropropan	13.65	157	6004	10.96	ppb	100
105) 1,2,4-Trichlorobenzene	14.56	180	41263	11.69	ppb	100
106) Hexachlorobutadiene	14.76	225	27458	12.69	ppb	100
107) Naphthalene	14.83	128	32656	10.32	ppb	100
108) 1,2,3-Trichlorobenzene	15.10	180	36307	10.98	ppb	100

Quantitation Report


Data File : M:\THOR\DATA\211109\1109T19.D  
Acq On : 9 Nov 21 13:52  
Sample : 10ug/L VOC STD 11/9/21  
Misc : IS&S 8/15/21

Vial: 7  
Operator:  
Inst : Thor  
Multiplr: 1.00

Quant Time: Nov 10 9:44 2021

Quant Results File: T1109W.RES

Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Wed Nov 10 10:21:13 2021  
Response via : Initial Calibration



Data File : M:\THOR\DATA\211109\1109T20.D  
 Acq On : 9 Nov 21 14:17  
 Sample : 20ug/L VOC STD 11/9/21  
 Misc : IS&S 8/15/21

Vial: 8  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 10 9:44 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 09:43:41 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.34	96	311782	25.00	ppb	0.00
68) Chlorobenzene-D5 (IS)	9.81	117	308423	25.00	ppb	0.00
83) 1,4-Dichlorobenzene-D (IS)	12.37	152	212717	25.00	ppb	0.00
System Monitoring Compounds						
43) Dibromofluoromethane(S)	5.49	111	190470	58.19	ppb	0.00
Spiked Amount	25.000		Recovery	=	232.744%	
48) 1,2-DCA-D4 (S)	5.91	65	203267	62.51	ppb	0.00
Spiked Amount	25.000		Recovery	=	250.056%	
69) Toluene-D8 (S)	8.22	98	649429	51.71	ppb	0.00
Spiked Amount	25.000		Recovery	=	206.828%	
77) 4-Bromofluorobenzene(S)	11.11	95	266888	54.96	ppb	0.00
Spiked Amount	25.000		Recovery	=	219.840%	
Target Compounds						
3) Dichlorodifluoromethane	1.09	85	18108	24.77	ppb	Qvalue 89
4) Freon 114	1.19	85	16018	21.48	ppb	93
5) Chloromethane	1.28	50	6632	15.25	ppb	95
6) Vinyl chloride	1.33	62	16565	15.06	ppb	96
7) Butane	1.59	43	149	143.88	ppb	# 100
9) Bromomethane	1.59	96	13437	17.56	ppb	100
10) Chloroethane	1.68	64	9181	16.38	ppb	# 86
11) Dichlorofluoromethane	1.87	67	35912	18.46	ppb	89
12) Trichlorofluoromethane	1.90	101	61050	24.57	ppb	97
16) Acrolein	2.31	56	25609	163.59	ppb	88
17) Acetone	2.48	43	18722	59.51	ppb	93
18) Freon-113	2.42	101	13268	20.55	ppb	98
19) 1,1-DCE	2.40	61	35117	20.65	ppb	91
21) Acetonitrile	2.79	40	2127	126.82	ppb	92
22) t-Butanol	3.16	59	5545	155.41	ppb	97
23) Methyl Acetate	2.87	43	11844	16.28	ppb	94
24) Iodomethane	2.55	142	13376	24.79	ppb	# 93
25) Acrylonitrile	3.29	52	4865	15.90	ppb	# 86
26) Methylene chloride	2.96	49	21618	16.58	ppb	91
27) Carbon disulfide	2.61	76	27536	18.15	ppb	99
28) Methyl t-butyl ether (MtBE)	3.34	73	66330	20.07	ppb	94
29) Trans-1,2-DCE	3.31	61	29813	19.13	ppb	98
31) Diisopropyl Ether	4.12	45	45361	15.28	ppb	87
33) 1,1-DCA	3.91	63	35949	17.96	ppb	95
34) Vinyl Acetate	4.11	43	36996	15.55	ppb	# 95
35) Ethyl tert Butyl Ether	4.67	59	59473	18.33	ppb	95
36) MEK (2-Butanone)	4.87	43	24934	56.04	ppb	92

(#) = qualifier out of range (m) = manual integration  
 1109T20.D T1109W.M Thu Nov 11 2021 13:51 2021



Quantitation Report (Not Reviewed)

Data File : M:\THOR\DATA\211109\1109T20.D  
 Acq On : 9 Nov 21 14:17  
 Sample : 20ug/L VOC STD 11/9/21  
 Misc : IS&S 8/15/21

Vial: 8  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 10 9:44 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 09:43:41 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
37) Cis-1,2-DCE	4.81	61	35512	18.69	ppb	97
38) 2,2-Dichloropropane	4.79	77	45560	21.78	ppb	95
39) 2-Methylpentane	3.17	43	3568	13.86	ppb	85
40) 3-Methylpentane	3.33	57	11912	18.36	ppb	86
41) Chloroform	5.28	83	52083	20.45	ppb	98
42) Bromochloromethane	5.13	49	14774	17.19	ppb	98
44) 1,1,1-TCA	5.49	97	24640	22.64	ppb	99
45) Cyclohexane	5.55	56	31966	17.80	ppb	93
46) 1,1-Dichloropropene	5.72	75	35655	20.19	ppb	97
47) 2,2,4-Trimethylpentane	6.13	57	70515	17.52	ppb	99
49) Carbon Tetrachloride	5.71	117	57753	25.25	ppb	99
50) Tert Amyl Methyl Ether	6.18	73	67704	18.64	ppb	96
51) Methylcyclopentane	4.67	56	3010	21.57	ppb	100
52) 1,2-DCA	6.01	62	41595	21.96	ppb	96
53) Benzene	5.97	78	95488	17.91	ppb	99
54) TCE	6.80	130	22224	21.41	ppb	96
55) 2-Pentanone	7.05	43	118799	136.76	ppb	97
56) 1,2-Dichloropropane	7.05	63	22463	16.41	ppb	# 96
57) Bromodichloromethane	7.40	83	40504	20.61	ppb	99
58) Methyl Cyclohexane	7.02	83	47101	19.84	ppb	96
59) Dibromomethane	7.19	174	37395	24.08	ppb	97
60) MIBK (methyl isobutyl ket	8.13	43	63384	52.88	ppb	95
61) 1-Bromo-2-chloroethane	7.73	63	14792	15.76	ppb	90
63) Cis-1,3-Dichloropropene	7.92	75	42901	19.45	ppb	95
64) Toluene	8.29	91	127247	18.73	ppb	97
65) Trans-1,3-Dichloropropene	8.56	75	41306	20.21	ppb	95
66) 1,1,2-TCA	8.75	97	27171	19.01	ppb	94
67) 2-Hexanone	9.06	43	44548	53.91	ppb	99
70) 1,2-EDB	9.28	107	31967	19.15	ppb	100
71) Tetrachloroethene	8.90	166	65699	22.77	ppb	98
72) 1-Chlorohexane	9.85	91	43347	17.94	ppb	98
73) 1,1,1,2-Tetrachloroethane	9.94	131	43070	21.39	ppb	89
74) m&p-Xylene	10.11	91	251528	39.31	ppb	99
75) o-Xylene	10.54	91	126119	19.29	ppb	99
76) Styrene	10.56	104	99152	19.39	ppb	99
78) 1,3-Dichloropropane	8.93	76	40184	17.13	ppb	99
79) Dibromochloromethane	9.17	129	43052	20.85	ppb	94
80) Chlorobenzene	9.84	112	102003	18.71	ppb	99
81) Ethylbenzene	9.98	91	153208	18.77	ppb	99
82) Bromoform	10.74	173	41552	23.44	ppb	99
84) Isopropylbenzene	10.95	105	171575	18.67	ppb	99
85) 1,1,2,2-Tetrachloroethane	11.27	83	34102	16.20	ppb	94

(#) = qualifier out of range (m) = manual integration

Data File : M:\THOR\DATA\211109\1109T20.D  
 Acq On : 9 Nov 21 14:17  
 Sample : 20ug/L VOC STD 11/9/21  
 Misc : IS&S 8/15/21

Vial: 8  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant. Time: Nov 10 9:44 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 09:43:41 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
86) 1,2,3-Trichloropropane	11.31	110	14416	19.01	ppb	# 88
87) t-1,4-Dichloro-2-Butene	11.34	53	7360	16.52	ppb	95
88) Bromobenzene	11.26	156	60751	20.15	ppb	90
89) n-Propylbenzene	11.40	91	181192	17.80	ppb	95
90) 4-Ethyltoluene	11.53	105	171199	19.35	ppb	98
91) 2-Chlorotoluene	11.48	91	123797	17.89	ppb	96
92) 1,3,5-Trimethylbenzene	11.60	105	148511	19.24	ppb	98
93) 4-Chlorotoluene	11.60	91	131816	18.74	ppb	99
94) Tert-Butylbenzene	11.95	119	162807	19.71	ppb	100
95) 1,2,4-Trimethylbenzene	12.00	105	147171	19.33	ppb	98
96) Sec-Butylbenzene	12.19	105	183063	18.71	ppb	99
97) p-Isopropyltoluene	12.35	119	175987	19.87	ppb	99
98) Benzyl Chloride	12.55	91	66909	18.10	ppb	99
99) 1,3-DCB	12.30	146	109381	20.13	ppb	99
100) 1,4-DCB	12.40	146	107342	19.46	ppb	98
101) n-Butylbenzene	12.80	91	127865	18.69	ppb	99
102) 1,2-DCB	12.80	146	98893	19.88	ppb	96
103) Hexachloroethane	13.09	201	43690	23.42	ppb	99
104) 1,2-Dibromo-3-chloropropan	13.65	157	12212	22.64	ppb	96
105) 1,2,4-Trichlorobenzene	14.56	180	78291	22.53	ppb	95
106) Hexachlorobutadiene	14.76	225	50790	23.84	ppb	96
107) Naphthalene	14.83	128	62736	20.13	ppb	98
108) 1,2,3-Trichlorobenzene	15.09	180	72047	22.12	ppb	93

Quantitation Report


Data File : M:\THOR\DATA\211109\1109T20.D  
Acq On : 9 Nov 21 14:17  
Sample : 20ug/L VOC STD 11/9/21  
Misc : IS&S 8/15/21

Vial: 8  
Operator:  
Inst : Thor  
Multiplr: 1.00

Quant Time: Nov 10 9:44 2021

Quant Results File: T1109W.RES

Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Wed Nov 10 10:21:13 2021  
Response via : Initial Calibration



Data File : M:\THOR\DATA\211109\1109T21.D  
 Acq On : 9 Nov 21 14:42  
 Sample : 40ug/L VOC STD 11/9/21  
 Misc : IS&S 8/15/21

Vial: 9  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 10 9:44 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 09:43:41 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.34	96	306148	25.00	ppb	0.00
68) Chlorobenzene-D5 (IS)	9.81	117	296587	25.00	ppb	0.00
83) 1,4-Dichlorobenzene-D (IS)	12.37	152	207105	25.00	ppb	0.00
System Monitoring Compounds						
43) Dibromofluoromethane(S)	5.49	111	194471	60.50	ppb	0.00
Spiked Amount	25.000		Recovery	=	242.004%	
48) 1,2-DCA-D4 (S)	5.91	65	204777	64.14	ppb	0.00
Spiked Amount	25.000		Recovery	=	256.548%	
69) Toluene-D8 (S)	8.22	98	651493	53.94	ppb	0.00
Spiked Amount	25.000		Recovery	=	215.764%	
77) 4-Bromofluorobenzene(S)	11.11	95	264443	56.63	ppb	0.00
Spiked Amount	25.000		Recovery	=	226.520%	
Target Compounds						
3) Dichlorodifluoromethane	1.09	85	37051	54.01	ppb	Qvalue 92
4) Freon 114	1.19	85	32802	45.74	ppb	99
5) Chloromethane	1.27	50	13156	30.80	ppb	99
6) Vinyl chloride	1.32	62	35322	32.69	ppb	94
7) Butane	1.59	43	41	40.32	ppb	# 100
9) Bromomethane	1.59	96	26799	35.67	ppb	96
10) Chloroethane	1.68	64	18531	33.67	ppb	# 89
11) Dichlorofluoromethane	1.86	67	74781	39.14	ppb	95
12) Trichlorofluoromethane	1.90	101	128692	52.75	ppb	98
16) Acrolein	2.31	56	29175	189.80	ppb	100
17) Acetone	2.47	43	24595	79.62	ppb	93
18) Freon-113	2.42	101	28824	45.47	ppb	98
19) 1,1-DCE	2.40	61	71748	43.05	ppb	# 88
21) Acetonitrile	2.78	40	2212	135.64	ppb	98
22) t-Butanol	3.17	59	5915	168.83	ppb	94
23) Methyl Acetate	2.86	43	25305	35.41	ppb	99
24) Iodomethane	2.54	142	26216	50.09	ppb	91
25) Acrylonitrile	3.28	52	10718	32.65	ppb	87
26) Methylene chloride	2.95	49	47648	37.49	ppb	97
27) Carbon disulfide	2.60	76	55952	37.56	ppb	100
28) Methyl t-butyl ether (MtBE)	3.33	73	142624	43.94	ppb	94
29) Trans-1,2-DCE	3.31	61	63183	41.28	ppb	97
31) Diisopropyl Ether	4.11	45	97208	33.35	ppb	88
33) 1,1-DCA	3.91	63	79910	40.65	ppb	96
34) Vinyl Acetate	4.11	43	90145	37.72	ppb	# 94
35) Ethyl tert Butyl Ether	4.67	59	127475	40.01	ppb	97
36) MEK (2-Butanone)	4.87	43	33949	77.70	ppb	100

(#) = qualifier out of range (m) = manual integration

Data File : M:\THOR\DATA\211109\1109T21.D  
 Acq On : 9 Nov 21 14:42  
 Sample : 40ug/L VOC STD 11/9/21  
 Misc : IS&S 8/15/21

Vial: 9  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 10 9:44 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 09:43:41 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
37) Cis-1,2-DCE	4.80	61	74814	40.10	ppb	96
38) 2,2-Dichloropropane	4.79	77	97513	47.48	ppb	99
39) 2-Methylpentane	3.17	43	3596	14.22	ppb #	81
40) 3-Methylpentane	3.33	57	25013	39.26	ppb #	82
41) Chloroform	5.28	83	111708	44.68	ppb	98
42) Bromochloromethane	5.13	49	29671	35.16	ppb	93
44) 1,1,1-TCA	5.49	97	52832	49.43	ppb	96
45) Cyclohexane	5.55	56	70281	39.86	ppb	95
46) 1,1-Dichloropropene	5.72	75	73741	42.51	ppb	97
47) 2,2,4-Trimethylpentane	6.13	57	152727	38.65	ppb	99
49) Carbon Tetrachloride	5.70	117	124198	55.29	ppb	100
50) Tert Amyl Methyl Ether	6.18	73	146613	41.10	ppb	93
51) Methylcyclopentane	4.67	56	5595	40.83	ppb	100
52) 1,2-DCA	6.00	62	86352	46.43	ppb #	93
53) Benzene	5.97	78	201078	38.41	ppb	98
54) TCE	6.80	130	47496	46.59	ppb	99
55) 2-Pentanone	7.05	43	133864	156.94	ppb	100
56) 1,2-Dichloropropane	7.05	63	48217	35.88	ppb #	95
57) Bromodichloromethane	7.40	83	88885	46.05	ppb	97
58) Methyl Cyclohexane	7.01	83	103414	44.37	ppb	91
59) Dibromomethane	7.18	174	81243	53.29	ppb	96
60) MIBK (methyl isobutyl ket	8.12	43	85039	72.25	ppb	95
61) 1-Bromo-2-chloroethane	7.73	63	31864	34.58	ppb #	88
62) 2-Chloroethyl vinyl ether	7.79	44	47	115.55	ppb	100
63) Cis-1,3-Dichloropropene	7.92	75	89897	41.51	ppb	95
64) Toluene	8.29	91	271249	40.65	ppb	99
65) Trans-1,3-Dichloropropene	8.56	75	90579	45.13	ppb	96
66) 1,1,2-TCA	8.75	97	57636	41.06	ppb	92
67) 2-Hexanone	9.06	43	62216	76.67	ppb	95
70) 1,2-EDB	9.29	107	68799	42.86	ppb	94
71) Tetrachloroethene	8.90	166	141732	51.08	ppb	96
72) 1-Chlorohexane	9.85	91	90449	38.93	ppb	99
73) 1,1,1,2-Tetrachloroethane	9.94	131	94918	49.02	ppb	91
74) m&p-Xylene	10.11	91	528959	85.56	ppb	98
75) o-Xylene	10.54	91	265515	42.23	ppb	100
76) Styrene	10.56	104	212926	43.30	ppb	99
78) 1,3-Dichloropropane	8.93	76	85448	37.87	ppb	96
79) Dibromochloromethane	9.17	129	93750	47.21	ppb	96
80) Chlorobenzene	9.84	112	215730	41.15	ppb	98
81) Ethylbenzene	9.98	91	329998	42.04	ppb	99
82) Bromoform	10.74	173	93518	54.87	ppb	96
84) Isopropylbenzene	10.95	105	360503	40.30	ppb	97

(#) = qualifier out of range (m) = manual integration

Data File : M:\THOR\DATA\211109\1109T21.D  
 Acq On : 9 Nov 21 14:42  
 Sample : 40ug/L VOC STD 11/9/21  
 Misc : IS&S 8/15/21

Vial: 9  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 10 9:44 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 09:43:41 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
85) 1,1,2,2-Tetrachloroethane	11.27	83	72618	35.43	ppb	96
86) 1,2,3-Trichloropropane	11.31	110	31498	42.65	ppb	92
87) t-1,4-Dichloro-2-Butene	11.34	53	17192	39.64	ppb	93
88) Bromobenzene	11.26	156	130236	44.37	ppb	97
89) n-Propylbenzene	11.40	91	387501	39.11	ppb	98
90) 4-Ethyltoluene	11.53	105	360655	41.87	ppb	97
91) 2-Chlorotoluene	11.48	91	268052	39.78	ppb	97
92) 1,3,5-Trimethylbenzene	11.60	105	314926	41.91	ppb	100
93) 4-Chlorotoluene	11.60	91	274184	40.05	ppb	98
94) Tert-Butylbenzene	11.95	119	335106	41.68	ppb	95
95) 1,2,4-Trimethylbenzene	12.00	105	313790	42.33	ppb	98
96) Sec-Butylbenzene	12.19	105	385603	40.49	ppb	98
97) p-Isopropyltoluene	12.35	119	375368	43.54	ppb	98
98) Benzyl Chloride	12.55	91	149362	41.50	ppb	100
99) 1,3-DCB	12.30	146	228009	43.09	ppb	97
100) 1,4-DCB	12.40	146	228671	42.58	ppb	98
101) n-Butylbenzene	12.80	91	271142	40.71	ppb	96
102) 1,2-DCB	12.80	146	211934	43.76	ppb	98
103) Hexachloroethane	13.09	201	94557	52.05	ppb	98
104) 1,2-Dibromo-3-chloropropan	13.65	157	27561	52.47	ppb	90
105) 1,2,4-Trichlorobenzene	14.57	180	171709	50.76	ppb	91
106) Hexachlorobutadiene	14.76	225	112832	54.39	ppb	95
107) Naphthalene	14.83	128	149120	49.15	ppb	100
108) 1,2,3-Trichlorobenzene	15.10	180	158954	50.13	ppb	94

# Quantitation Report


Data File : M:\THOR\DATA\211109\1109T21.D  
 Acq On : 9 Nov 21 14:42  
 Sample : 40ug/L VOC STD 11/9/21  
 Misc : IS&S 8/15/21

Vial: 9  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 10 9:44 2021

Quant Results File: T1109W.RES

Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 10:21:13 2021  
 Response via : Initial Calibration



Data File : M:\THOR\DATA\211109\1109T22.D  
 Acq On : 9 Nov 21 15:07  
 Sample : 100ug/L VOC STD 11/9/21  
 Misc : IS&S 8/15/21

Vial: 10  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 10 9:44 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 09:43:41 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.34	96	311870	25.00	ppb	0.00
68) Chlorobenzene-D5 (IS)	9.81	117	300158	25.00	ppb	0.00
83) 1,4-Dichlorobenzene-D (IS)	12.37	152	206230	25.00	ppb	0.00

System Monitoring Compounds

43) Dibromofluoromethane(S)	5.49	111	392992	120.02	ppb	0.00
Spiked Amount	25.000		Recovery	=	480.076%	
48) 1,2-DCA-D4(S)	5.90	65	420171	129.19	ppb	0.00
Spiked Amount	25.000		Recovery	=	516.740%	
69) Toluene-D8(S)	8.22	98	1311557	107.30	ppb	0.00
Spiked Amount	25.000		Recovery	=	429.204%	
77) 4-Bromofluorobenzene(S)	11.11	95	522234	110.51	ppb	0.00
Spiked Amount	25.000		Recovery	=	442.020%	

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Dichlorodifluoromethane	1.09	85	52696	76.28	ppb	96
4) Freon 114	1.19	85	54761	75.52	ppb	83
5) Chloromethane	1.27	50	31475	72.34	ppb	98
6) Vinyl chloride	1.32	62	85227	77.44	ppb	88
7) Butane	1.60	43	628	606.25	ppb #	100
9) Bromomethane	1.58	96	62279	81.38	ppb	94
10) Chloroethane	1.67	64	37619	67.09	ppb #	82
11) Dichlorofluoromethane	1.86	67	159199	81.80	ppb	93
12) Trichlorofluoromethane	1.90	101	277174	111.52	ppb	99
16) Acrolein	2.31	56	33320	212.79	ppb	98
17) Acetone	2.48	43	30243	96.11	ppb	97
18) Freon-113	2.42	101	71208	110.28	ppb	99
19) 1,1-DCE	2.40	61	182800	107.77	ppb	92
21) Acetonitrile	2.79	40	2364	143.60	ppb	99
22) t-Butanol	3.17	59	5315	148.92	ppb	98
23) Methyl Acetate	2.86	43	68100	93.56	ppb	93
24) Iodomethane	2.54	142	51224	96.63	ppb	96
25) Acrylonitrile	3.27	52	28516	81.36	ppb #	86
26) Methylene chloride	2.95	49	114950	89.09	ppb #	90
27) Carbon disulfide	2.60	76	129008	85.02	ppb	100
28) Methyl t-butyl ether (MtBE)	3.33	73	370414	112.03	ppb	93
29) Trans-1,2-DCE	3.30	61	158474	101.65	ppb	95
31) Diisopropyl Ether	4.11	45	250218	84.27	ppb	81
33) 1,1-DCA	3.91	63	201296	100.51	ppb	94
34) Vinyl Acetate	4.11	43	237305	96.52	ppb #	92
35) Ethyl tert Butyl Ether	4.67	59	322791	99.46	ppb	97
36) MEK (2-Butanone)	4.87	43	42327	95.10	ppb	98

(#) = qualifier out of range (m) = manual integration



Data File : M:\THOR\DATA\211109\1109T22.D  
 Acq On : 9 Nov 21 15:07  
 Sample : 100ug/L VOC STD 11/9/21  
 Misc : IS&S 8/15/21

Vial: 10  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 10 9:44 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 09:43:41 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
37) Cis-1,2-DCE	4.80	61	191813	100.93	ppb	95
38) 2,2-Dichloropropane	4.79	77	242560	115.95	ppb	99
39) 2-Methylpentane	3.18	43	4398	17.07	ppb	92
40) 3-Methylpentane	3.33	57	66410	102.32	ppb	# 83
41) Chloroform	5.28	83	278211	109.23	ppb	98
42) Bromochloromethane	5.13	49	74515	86.69	ppb	87
44) 1,1,1-TCA	5.49	97	132736	121.92	ppb	98
45) Cyclohexane	5.55	56	175491	97.69	ppb	# 87
46) 1,1-Dichloropropene	5.71	75	190691	107.92	ppb	98
47) 2,2,4-Trimethylpentane	6.13	57	389035	96.64	ppb	98
49) Carbon Tetrachloride	5.70	117	322619	140.99	ppb	97
50) Tert Amyl Methyl Ether	6.18	73	372223	102.44	ppb	94
51) Methylcyclopentane	4.67	56	13914	99.67	ppb	# 100
52) 1,2-DCA	6.00	62	215796	113.90	ppb	95
53) Benzene	5.97	78	506790	95.02	ppb	99
54) TCE	6.79	130	123656	119.08	ppb	98
55) 2-Pentanone	7.05	43	159804	183.92	ppb	97
56) 1,2-Dichloropropane	7.05	63	117662	85.94	ppb	# 95
57) Bromodichloromethane	7.40	83	227209	115.56	ppb	99
58) Methyl Cyclohexane	7.01	83	257043	108.26	ppb	97
59) Dibromomethane	7.18	174	207034	133.30	ppb	98
60) MIBK (methyl isobutyl ket	8.12	43	112498	93.83	ppb	94
61) 1-Bromo-2-chloroethane	7.73	63	83072	88.49	ppb	# 89
63) Cis-1,3-Dichloropropene	7.92	75	233147	105.69	ppb	95
64) Toluene	8.29	91	681615	100.29	ppb	97
65) Trans-1,3-Dichloropropene	8.56	75	231896	113.42	ppb	98
66) 1,1,2-TCA	8.75	97	146076	102.15	ppb	92
67) 2-Hexanone	9.06	43	80851	97.81	ppb	94
70) 1,2-EDB	9.28	107	174811	107.60	ppb	96
71) Tetrachloroethene	8.90	166	347390	123.72	ppb	99
72) 1-Chlorohexane	9.85	91	227252	96.64	ppb	99
73) 1,1,1,2-Tetrachloroethane	9.94	131	238210	121.57	ppb	97
74) m&p-Xylene	10.11	91	1305959	208.21	ppb	98
75) o-Xylene	10.54	91	666355	104.72	ppb	99
76) Styrene	10.56	104	536319	107.77	ppb	99
78) 1,3-Dichloropropane	8.93	76	215929	94.57	ppb	97
79) Dibromochloromethane	9.17	129	239614	119.24	ppb	95
80) Chlorobenzene	9.84	112	538718	101.54	ppb	99
81) Ethylbenzene	9.98	91	816414	102.76	ppb	100
82) Bromoform	10.74	173	235277	136.40	ppb	100
84) Isopropylbenzene	10.95	105	892573	100.20	ppb	96
85) 1,1,2,2-Tetrachloroethane	11.27	83	178280	87.36	ppb	94

(#) = qualifier out of range (m) = manual integration

Data File : M:\THOR\DATA\211109\1109T22.D  
 Acq On : 9 Nov 21 15:07  
 Sample : 100ug/L VOC STD 11/9/21  
 Misc : IS&S 8/15/21

Vial: 10  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 10 9:44 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 09:43:41 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
86) 1,2,3-Trichloropropane	11.31	110	75538	102.73	ppb	96
87) t-1,4-Dichloro-2-Butene	11.34	53	46559	107.82	ppb	94
88) Bromobenzene	11.26	156	318566	108.98	ppb	97
89) n-Propylbenzene	11.40	91	957499	97.05	ppb	96
90) 4-Ethyltoluene	11.53	105	890703	103.85	ppb	98
91) 2-Chlorotoluene	11.48	91	647311	96.47	ppb	94
92) 1,3,5-Trimethylbenzene	11.60	105	768644	102.72	ppb	99
93) 4-Chlorotoluene	11.60	91	669193	98.15	ppb	100
94) Tert-Butylbenzene	11.95	119	825063	103.04	ppb	96
95) 1,2,4-Trimethylbenzene	12.00	105	768648	104.12	ppb	98
96) Sec-Butylbenzene	12.19	105	959959	101.23	ppb	97
97) p-Isopropyltoluene	12.36	119	915310	106.61	ppb	98
98) Benzyl Chloride	12.55	91	388074	108.28	ppb	100
99) 1,3-DCB	12.30	146	554972	105.33	ppb	97
100) 1,4-DCB	12.40	146	554138	103.62	ppb	100
101) n-Butylbenzene	12.80	91	685906	103.42	ppb	98
102) 1,2-DCB	12.80	146	521275	108.09	ppb	99
103) Hexachloroethane	13.09	201	244998	135.44	ppb	93
104) 1,2-Dibromo-3-chloropropan	13.65	157	74271	142.00	ppb	98
105) 1,2,4-Trichlorobenzene	14.56	180	452860	134.45	ppb	90
106) Hexachlorobutadiene	14.76	225	278381	134.75	ppb	95
107) Naphthalene	14.83	128	407744	134.95	ppb	100
108) 1,2,3-Trichlorobenzene	15.10	180	412542	130.65	ppb	93

Quantitation Report


Data File : M:\THOR\DATA\211109\1109T22.D  
Acq On : 9 Nov 21 15:07  
Sample : 100ug/L VOC STD 11/9/21  
Misc : IS&S 8/15/21

Vial: 10  
Operator:  
Inst : Thor  
Multiplr: 1.00

Quant Time: Nov 10 9:44 2021

Quant Results File: T1109W.RES

Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Wed Nov 10 10:21:13 2021  
Response via : Initial Calibration



VOLATILE ORGANIC ANALYSIS  
VOLATILE ORGANIC COMPOUNDS

Form 7

Second Source Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Date Analyzed: 9 Nov 21 15:57  
Instrument: Thor  
Initial Cal. Date: 11/9/2021  
Data File: 1109T24.D

		Compound	MEAN	CCRF	%D	%Drift	
1	TML	Dichlorodifluoromethane	0.0890	0.0986	11	TML	28 *High
2	TMQ	Freon 114	0.0545	0.0969	78	TMQ	45 *High
3	TM**L	Chloromethane	0.0330	0.0287	13	TM**L	7.2
4	TM*L	Vinyl chloride	0.0684	0.0751	9.9	TM*L	8.9
5	TML	Bromomethane	0.0607	0.0587	3.4	TML	8.1
6	TML	Chloroethane	0.0340	0.0391	15	TML	7.2
7	TML	Dichlorofluoromethane	0.1408	0.1540	9.4	TML	6.9
8	TM	Trichlorofluoromethane	0.2378	0.2353	1.0	TM	
9	TM	Acrolein	0.0124	0.0137	10	TM	
10	TM	Acetone	0.0235	0.0266	13	TM	
11	TM	Freon-113	0.0568	0.0517	9.0	TM	
12	TM*L	1,1-DCE	0.1398	0.1362	2.6	TM*L	5.3
13	TMQ	Acetonitrile	0.0012	0.0014	18	TMQ	38 *High
14	TM	t-Butanol	0.0032	0.0035	12	TM	
15	TML	Methyl Acetate	0.0417	0.0468	12	TML	1.5
16	TML	Iodomethane	0.0622	0.0607	2.5	TML	11
17	TML	Acrylonitrile	0.0146	0.0170	16	TML	2.7
18	TML	Methylene chloride	0.0836	0.0948	13	TML	2.8
19	TML	Carbon disulfide	0.1230	0.1172	4.7	TML	4.7
20	TM	Methyl t-butyl ether (MtBE)	0.2625	0.2686	2.4	TM	
21	TML	Trans-1,2-DCE	0.1081	0.1119	3.5	TML	8.4
22	TML	Diisopropyl Ether	0.1643	0.1818	11	TML	3.9
23	TM**L	1,1-DCA	0.1390	0.1480	6.5	TM**L	3.1
24	TML	Vinyl Acetate	0.1294	0.1415	9.3	TML	12
25	TM	Ethyl tert Butyl Ether	0.2262	0.2432	7.5	TM	
26	TM	MEK (2-Butanone)	0.0302	0.0336	11	TM	
27	TM	Cis-1,2-DCE	0.1314	0.1456	11	TM	
28	TM	2,2-Dichloropropane	0.1719	0.1830	6.4	TM	
29	TM	2-Methylpentane	0.0000	0.0236	0.00	TM	
30	TML	3-Methylpentane	0.0432	0.0449	3.8	TML	7.6
31	TM*	Chloroform	0.2008	0.2100	4.6	TM*	
32	TML	Bromochloromethane	0.0543	0.0618	14	TML	4.3
33	TM	1,1,1-TCA	0.1032	0.1009	2.2	TM	
34	TML	Cyclohexane	0.1195	0.1232	3.2	TML	7.9
35	TML	1,1-Dichloropropene	0.1338	0.1410	5.4	TML	2.9
36	TM	2,2,4-Trimethylpentane	0.2757	0.2677	2.9	TM	
37	TML	Carbon Tetrachloride	0.2081	0.2290	10	TML	4.1
38	TM	Tert Amyl Methyl Ether	0.2710	0.2731	0.77	TM	
39	TML	Methylcyclopentane	0.0097	0.0086	11	TML	21 *NT
40	TM	1,2-DCA	0.1699	0.1713	0.83	TM	
Average					9.5		

VOLATILE ORGANIC ANALYSIS  
VOLATILE ORGANIC COMPOUNDS

Form 7

Second Source Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Date Analyzed: 9 Nov 21 15:57  
Instrument: Thor  
Cal. Date: 11/9/2021  
Data File: 1109T24.D

		Compound	MEAN	CCRF	%D	%Drift
41	TM	Benzene	0.3968	0.3838	3.3	TM
42	TM	TCE	0.0925	0.0857	7.3	TM
43	TM	2-Pentanone	0.0618	0.0676	9.5	TM
44	TM*	1,2-Dichloropropane	0.0895	0.0922	3.0	TM*
45	TM	Bromodichloromethane	0.1636	0.1630	0.39	TM
46	TM	Methyl Cyclohexane	0.1835	0.1880	2.4	TM
47	TML	Dibromomethane	0.1451	0.1558	7.4	TML 1.5
48	TM	MIBK (methyl isobutyl ketone)	0.0804	0.0874	8.7	TM
49	TM	1-Bromo-2-chloroethane	0.0627	0.0601	4.1	TM
50	TM	Cis-1,3-Dichloropropene	0.1668	0.1645	1.4	TM
51	TM*	Toluene	0.5221	0.5233	0.21	TM*
52	TM	Trans-1,3-Dichloropropene	0.1616	0.1631	0.89	TM
53	TML	1,1,2-TCA	0.1058	0.1155	9.1	TML 2.0
54	TM	2-Hexanone	0.0563	0.0601	6.7	TM
55	TM	1,2-EDB	0.1292	0.1336	3.4	TM
56	TM	Tetrachloroethene	0.2793	0.2752	1.5	TM
57	TML	1-Chlorohexane	0.1924	0.1718	11	TML 6.9
58	TM	1,1,1,2-Tetrachloroethane	0.1799	0.1769	1.7	TM
59	TM	m&p-Xylene	0.5028	0.5039	0.22	TM
60	TM	o-Xylene	0.5296	0.5171	2.4	TM
61	TM	Styrene	0.3906	0.3856	1.3	TM
62	TM	1,3-Dichloropropane	0.1660	0.1694	2.1	TM
63	TM	Dibromochloromethane	0.1778	0.1742	2.1	TM
64	TM**	Chlorobenzene	0.4416	0.4195	5.0	TM**
65	TM*	Ethylbenzene	0.6541	0.6194	5.3	TM*
66	TM**	Bromoform	0.1722	0.1695	1.5	TM**
67	TM	Isopropylbenzene	0.9854	1.004	1.9	TM
68	TM**	1,1,2,2-Tetrachloroethane	0.1957	0.2002	2.3	TM**
69	TML	1,2,3-Trichloropropane	0.0863	0.0890	3.2	TML 0.93
70	TML	t-1,4-Dichloro-2-Butene	0.0434	0.0491	13	TML 3.9
71	TM	Bromobenzene	0.3619	0.3634	0.41	TM
72	TM	n-Propylbenzene	1.085	1.045	3.7	TM
73	TM	4-Ethyltoluene	1.007	0.9875	1.9	TM
74	TM	2-Chlorotoluene	0.7393	0.7254	1.9	TM
75	TM	1,3,5-Trimethylbenzene	0.8976	0.8761	2.4	TM
76	TM	4-Chlorotoluene	0.7492	0.7657	2.2	TM
77	TM	Tert-Butylbenzene	0.9345	0.9275	0.75	TM
78	TM	1,2,4-Trimethylbenzene	0.8548	0.8698	1.8	TM
79	TM	Sec-Butylbenzene	1.079	1.039	3.7	TM
80	TM	p-Isopropyltoluene	1.023	1.009	1.3	TM
		Average			3.6	

VOLATILE ORGANIC ANALYSIS  
VOLATILE ORGANIC COMPOUNDS

Form 7

Second Source Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Date Analyzed: 9 Nov 21 15:57  
Instrument: Thor  
Cal. Date: 11/9/2021  
Data File: 1109T24.D

		Compound	MEAN	CCRF	%D	%Drift
81	TM	Benzyl Chloride	0.3838	0.3431	11	TM
82	TM	1,3-DCB	0.6603	0.6479	1.9	TM
83	TM	1,4-DCB	0.6822	0.6669	2.2	TM
84	TM	n-Butylbenzene	0.7192	0.7208	0.22	TM
85	TM	1,2-DCB	0.6039	0.5898	2.3	TM
86	TML	Hexachloroethane	0.2240	0.2529	13	TML 5.6
87	TML	1,2-Dibromo-3-chloropropane	0.0586	0.0669	14	TML 11
88	TML	1,2,4-Trichlorobenzene	0.4679	0.4552	2.7	TML 6.6
89	TM	Hexachlorobutadiene	0.3204	0.3066	4.3	TM
90	TML	Naphthalene	0.3777	0.3827	1.3	TML 6.5
91	TM	1,2,3-Trichlorobenzene	0.4252	0.4225	0.64	TM
92						
93						
94						
95						
96						
97						
98						
99						
100						
101						
102						
103						
104						
105						
106						
107						
108						
109						
110						
111						
112						
113						
114						
115						
116						
117						
118						
119						
120						

Average

4.9

Data File : M:\THOR\DATA\211109\1109T24.D  
 Acq On : 9 Nov 21 15:57  
 Sample : (SS) 10ug/L VOC STD 11/9/21  
 Misc : IS&S 8/15/21

Vial: 12  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 10 10:21 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 10:21:13 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.34	96	310765	25.00	ppb	0.00
68) Chlorobenzene-D5 (IS)	9.81	117	306633	25.00	ppb	0.00
83) 1,4-Dichlorobenzene-D (IS)	12.37	152	215446	25.00	ppb	0.00

System Monitoring Compounds

43) Dibromofluoromethane(S)	5.49	111	91737	26.38	ppb	0.00
Spiked Amount	25.000		Recovery	= 105.524%		
48) 1,2-DCA-D4(S)	5.91	65	98369	26.43	ppb	0.00
Spiked Amount	25.000		Recovery	= 105.712%		
69) Toluene-D8(S)	8.22	98	318747	26.43	ppb	0.00
Spiked Amount	25.000		Recovery	= 105.732%		
77) 4-Bromofluorobenzene(S)	11.11	95	129023	26.81	ppb	0.00
Spiked Amount	25.000		Recovery	= 107.236%		

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Dichlorodifluoromethane	1.09	85	12262	12.82	ppb	93
4) Freon 114	1.19	85	12049	14.51	ppb	81
5) Chloromethane	1.26	50	3570	10.72	ppb #	85
6) Vinyl chloride	1.32	62	9340	10.89	ppb	95
9) Bromomethane	1.58	96	7292	10.81	ppb	91
10) Chloroethane	1.67	64	4865	10.72	ppb	93
11) Dichlorofluoromethane	1.86	67	19139	10.69	ppb	97
12) Trichlorofluoromethane	1.90	101	29245	9.90	ppb	94
16) Acrolein	2.30	56	21257	138.00	ppb	99
17) Acetone	2.47	43	16517	56.57	ppb	96
18) Freon-113	2.42	101	6423	9.10	ppb	97
19) 1,1-DCE	2.40	61	16925	9.47	ppb #	86
21) Acetonitrile	2.77	40	2224	172.85	ppb	98
22) t-Butanol	3.16	59	5500	140.29	ppb	95
23) Methyl Acetate	2.86	43	5823	10.15	ppb	89
24) Iodomethane	2.54	142	7544	11.08	ppb	98
25) Acrylonitrile	3.30	52	2116	10.27	ppb	90
26) Methylene chloride	2.95	49	11786	10.28	ppb #	79
27) Carbon disulfide	2.60	76	14573	10.47	ppb	98
28) Methyl t-butyl ether (MtBE)	3.33	73	33393	10.24	ppb	93
29) Trans-1,2-DCE	3.31	61	13906	9.16	ppb	93
31) Diisopropyl Ether	4.11	45	22601	9.61	ppb	97
33) 1,1-DCA	3.92	63	18402	9.69	ppb	98
34) Vinyl Acetate	4.11	43	17587	8.77	ppb	98
35) Ethyl tert Butyl Ether	4.67	59	30231	10.75	ppb	87
36) MEK (2-Butanone)	4.87	43	20871	55.66	ppb	96
37) Cis-1,2-DCE	4.81	61	18101	11.09	ppb	89

(#) = qualifier out of range (m) = manual integration

Data File : M:\THOR\DATA\211109\1109T24.D  
 Acq On : 9 Nov 21 15:57  
 Sample : (SS) 10ug/L VOC STD 11/9/21  
 Misc : IS&S 8/15/21

Vial: 12  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 10 10:21 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 10:21:13 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
38) 2,2-Dichloropropane	4.79	77	22743	10.64	ppb	91
40) 3-Methylpentane	3.33	57	5580	9.24	ppb	# 94
41) Chloroform	5.28	83	26109	10.46	ppb	95
42) Bromochloromethane	5.13	49	7676	10.43	ppb	90
44) 1,1,1-TCA	5.49	97	12540	9.78	ppb	# 92
45) Cyclohexane	5.55	56	15319	9.21	ppb	95
46) 1,1-Dichloropropene	5.72	75	17525	9.71	ppb	94
47) 2,2,4-Trimethylpentane	6.13	57	33280	9.71	ppb	98
49) Carbon Tetrachloride	5.70	117	28467	9.59	ppb	92
50) Tert Amyl Methyl Ether	6.18	73	33944	10.08	ppb	92
51) Methylcyclopentane	4.67	56	1067	7.91	ppb	100
52) 1,2-DCA	6.01	62	21294	10.08	ppb	99
53) Benzene	5.97	78	47706	9.67	ppb	99
54) TCE	6.80	130	10654	9.27	ppb	95
55) 2-Pentanone	7.05	43	105110	136.89	ppb	100
56) 1,2-Dichloropropane	7.05	63	11459	10.30	ppb	# 94
57) Bromodichloromethane	7.40	83	20262	9.96	ppb	93
58) Methyl Cyclohexane	7.02	83	23372	10.24	ppb	95
59) Dibromomethane	7.19	174	19364	9.85	ppb	99
60) MIBK (methyl isobutyl ket	8.12	43	54304	54.33	ppb	95
61) 1-Bromo-2-chloroethane	7.73	63	7471	9.59	ppb	# 86
63) Cis-1,3-Dichloropropene	7.92	75	20454	9.86	ppb	# 87
64) Toluene	8.29	91	65045	10.02	ppb	99
65) Trans-1,3-Dichloropropene	8.56	75	20269	10.09	ppb	99
66) 1,1,2-TCA	8.75	97	14357	10.20	ppb	92
67) 2-Hexanone	9.06	43	37371	53.36	ppb	91
70) 1,2-EDB	9.29	107	16383	10.34	ppb	100
71) Tetrachloroethene	8.90	166	33760	9.85	ppb	95
72) 1-Chlorohexane	9.85	91	21070	9.31	ppb	96
73) 1,1,1,2-Tetrachloroethane	9.94	131	21692	9.83	ppb	96
74) m&p-Xylene	10.11	91	123598	20.04	ppb	99
75) o-Xylene	10.54	91	63426	9.76	ppb	98
76) Styrene	10.56	104	47291	9.87	ppb	99
78) 1,3-Dichloropropane	8.93	76	20779	10.21	ppb	99
79) Dibromochloromethane	9.18	129	21361	9.79	ppb	90
80) Chlorobenzene	9.85	112	51452	9.50	ppb	94
81) Ethylbenzene	9.98	91	75969	9.47	ppb	99
82) Bromoform	10.74	173	20792	9.85	ppb	97
84) Isopropylbenzene	10.95	105	86564	10.19	ppb	98
85) 1,1,2,2-Tetrachloroethane	11.27	83	17249	10.23	ppb	94
86) 1,2,3-Trichloropropane	11.31	110	7669	9.91	ppb	# 83
87) t-1,4-Dichloro-2-Butene	11.34	53	4230	10.39	ppb	89

(#) = qualifier out of range (m) = manual integration



Data File : M:\THOR\DATA\211109\1109T24.D  
 Acq On : 9 Nov 21 15:57  
 Sample : (SS) 10ug/L VOC STD 11/9/21  
 Misc : IS&S 8/15/21

Vial: 12  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 10 10:21 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 10:21:13 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
88) Bromobenzene	11.26	156	31319	10.04	ppb	96
89) n-Propylbenzene	11.40	91	90038	9.63	ppb	96
90) 4-Ethyltoluene	11.53	105	85105	9.81	ppb	97
91) 2-Chlorotoluene	11.48	91	62512	9.81	ppb	99
92) 1,3,5-Trimethylbenzene	11.60	105	75498	9.76	ppb	98
93) 4-Chlorotoluene	11.60	91	65985	10.22	ppb	97
94) Tert-Butylbenzene	11.95	119	79931	9.92	ppb	95
95) 1,2,4-Trimethylbenzene	12.00	105	74960	10.18	ppb	98
96) Sec-Butylbenzene	12.19	105	89545	9.63	ppb	99
97) p-Isopropyltoluene	12.35	119	86987	9.87	ppb	97
98) Benzyl Chloride	12.55	91	29567	8.94	ppb	96
99) 1,3-DCB	12.30	146	55838	9.81	ppb	96
100) 1,4-DCB	12.40	146	57474	9.78	ppb	97
101) n-Butylbenzene	12.80	91	62116	10.02	ppb	99
102) 1,2-DCB	12.80	146	50830	9.77	ppb	98
103) Hexachloroethane	13.09	201	21796	9.44	ppb	93
104) 1,2-Dibromo-3-chloropropan	13.65	157	5768	8.88	ppb	96
105) 1,2,4-Trichlorobenzene	14.56	180	39226	9.34	ppb	93
106) Hexachlorobutadiene	14.76	225	26419	9.57	ppb	92
107) Naphthalene	14.83	128	32984	9.35	ppb	98
108) 1,2,3-Trichlorobenzene	15.10	180	36409	9.94	ppb	96

Quantitation Report


Data File : M:\THOR\DATA\211109\1109T24.D  
Acq On : 9 Nov 21 15:57  
Sample : (SS) 10ug/L VOC STD 11/9/21  
Misc : IS&S 8/15/21

Vial: 12  
Operator:  
Inst : Thor  
Multiplr: 1.00

Quant Time: Nov 10 10:21 2021

Quant Results File: T1109W.RES

Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Wed Nov 10 10:21:13 2021  
Response via : Initial Calibration



VOLATILE ORGANIC ANALYSIS BY  
EPA METHOD 8260B

**Form 6**  
**Initial Calibration**

Lab Name: APPL, Inc.

SDG No: \_\_\_\_\_

Case No: \_\_\_\_\_

Initial Cal. Date: 11/11/2021

Matrix: Water

Instrument: Max

Initials: PA

1111M22.D    1111M23.D    1111M24.D    1111M25.D    1111M26.D    1111M27.D    1111M28.D    1111M29.D    1111M30.D

	Compound	1	2	3	4	5	6	7	8	9		Avg	%RSD	Type	r^2	Q	MRF
1	I	Fluorobenzene (IS)															
2	TM	Chlorotrifluoroethene												TM			
3	TM	Dichlorodifluoromethane	0.1582	0.1063	0.1229	0.1502	0.1056	0.1433	0.1387	0.1398	0.1412	0.13	14	TM			
4	TM	Freon 114		0.0917	0.0744	0.1084	0.0821	0.0931	0.0915	0.0937	0.0939	0.09	11	TM			
5	TM**	Chloromethane	0.1121	0.1127	0.0790	0.0991	0.0732	0.0822	0.0700	0.0792	0.0777	0.09	19	TM**	0.998		
6	TM*	Vinyl chloride		0.1042	0.1114	0.0926	0.0833	0.0823	0.0903	0.0889	0.0886	0.09	11	TM*			
7	TM	2-Chloro-1,1,1-trifluoroethane												TM			
8	TM	Bromomethane	0.1164	0.1289	0.0902	0.1244	0.0986	0.0969	0.0935	0.0907	0.0887	0.10	15	TM			
9	TML	Chloroethane	0.1537	0.1121	0.0922	0.0955	0.0746	0.0671	0.0572	0.0570		0.09	37	TM	0.998		
10	TM	Dichlorofluoromethane	0.1978	0.1917	0.1935	0.2084	0.2089	0.2252	0.2106	0.2211	0.2111	0.21	5.5	TM			
11	TM	Trichlorofluoromethane	0.1743	0.2514	0.2631	0.3059	0.2608	0.2970	0.2789	0.2864	0.2722	0.27	14	TM			
12	TM	2,2-Dichloro-1,1,1-trifluoroethane												TM			
13	TM	Acrolein	0.0127	0.0113	0.0124	0.0124	0.0111	0.0109	0.0114	0.0114	0.0115	0.01	5.5	TM			
14	TM	Acetone	0.0334	0.0306	0.0294	0.0290	0.0286	0.0297	0.0298	0.0294	0.0309	0.03	4.7	TM			
15	TM	Freon-113	0.0804	0.1028	0.1281	0.1353	0.1249	0.1257	0.1164	0.1236	0.1159	0.12	14	TM			
16	TM	Acetonitrile	0.0087	0.0070	0.0074	0.0069	0.0073	0.0075	0.0074	0.0076	0.0078	0.01	7.1	TM			
17	TML	2-propanol												TM			
18	TM	1,2-Dichlorotrifluoroethane	0.1978	0.1917	0.1935	0.2084	0.2089	0.2252	0.2106	0.2211	0.2111	0.21	5.5	TM			
19	TM*L	1,1-DCE	0.0984	0.1286	0.1851	0.1594	0.1436	0.1641	0.1555	0.1610	0.1586	0.15	16	TM*	1.000		
20	TM	t-Butanol	0.0117	0.0095	0.0093	0.0103	0.0106	0.0098	0.0098	0.0123		0.01	10	TM			
21	TM	Methyl Acetate	0.0495	0.0578	0.0493	0.0524	0.0533	0.0514	0.0449	0.0496	0.0474	0.05	7.3	TM			
22	TML	Iodomethane	0.0644	0.0803	0.1026	0.1089	0.0993	0.1196	0.1265	0.1445	0.1473	0.11	25	TM	0.999		
23	TML	Acrylonitrile	0.0038	0.0147	0.0254	0.0286	0.0269	0.0288	0.0278	0.0283	0.0272	0.02	37	TM	1.000		
24	TML	2-Methylpentane												TM			
25	TML	Methylene chloride		0.0585	0.0660	0.1056	0.0992	0.1040	0.1009	0.1017	0.0997	0.09	20	TM	1.000		
26	TM	Carbon disulfide	0.1170	0.1289	0.1337	0.1320	0.1267	0.1248	0.1167	0.1250	0.1120	0.12	6.0	TM			
27	TML	Methyl t-butyl ether (MtBE)	0.1854	0.3828	0.3082	0.3574	0.3625	0.3605	0.3385	0.3612	0.3273	0.33	18	TM	0.998		
28	TM	Trans-1,2-DCE	0.0798	0.1169	0.1120	0.0968	0.1078	0.1086	0.1052	0.1100	0.1042	0.10	10	TM			
29	TM	3-Methylpentane	0.0875	0.0619	0.0829	0.0558	0.0561	0.0575	0.0566	0.0601	0.0543	0.06	20	TM	0.998		
30	TM	Hexane												TM			
31	TM	Diisopropyl Ether	0.1759	0.1391	0.2210	0.2330	0.2281	0.2247	0.2247	0.2338	0.2258	0.21	15	TM			
32	TM**	1,1-DCA	0.1454	0.1432	0.2014	0.1930	0.1749	0.1854	0.1765	0.1775	0.1684	0.17	11	TM**			
33	TM	Vinyl Acetate												TM			
34	TM	Ethyl tert Butyl Ether	0.2765	0.2891	0.2692	0.3049	0.2933	0.2823	0.2693	0.2846	0.2679	0.28	4.5	TM			
35	TML	Methylcyclopentane				0.0130	0.0127	0.0137	0.0129	0.0114	0.0105	0.01	9.5	TM	0.998		

VOLATILE ORGANIC ANALYSIS BY  
EPA METHOD 8260B

Form 6  
Initial Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Initial Cal. Date: 11/11/2021  
Instrument: Max

Initials: PA

		Compound	1	2	3	4	5	6	7	8	9		Avg	%RSD	Type	Q	MRF
36	TM	MEK (2-Butanone)	0.0384	0.0311	0.0302	0.0348	0.0322	0.0308	0.0311	0.0315	0.0316		0.03	8.0	TM		
37	TML	Cis-1,2-DCE	0.0570	0.1140	0.1354	0.1450	0.1324	0.1233	0.1282	0.1250	0.1201		0.12	21	TM	1.000	
38	TM	2,2-Dichloropropane	0.1733	0.2499	0.2508	0.2593	0.2146	0.2434	0.2196	0.2259	0.2129		0.23	12	TM		
39	TM*	Chloroform	0.1909	0.2713	0.2360	0.2606	0.2547	0.2436	0.2419	0.2487	0.2374		0.24	9.3	TM*		
40	TML	Bromochloromethane	0.0612	0.1143	0.1032	0.1178	0.1064	0.1064	0.1015	0.1004	0.0965		0.10	16	TM	1.000	
41	S	Dibromofluoromethane(S)	0.3428	0.3337	0.2948	0.2986	0.3078	0.3132	0.3127	0.3158	0.2850		0.31	5.8	S		
42	TML	1,1,1-TCA	0.1485	0.2917	0.2837	0.3024	0.2812	0.2793	0.2790	0.2818	0.2641		0.27	17	TM	0.999	
43	TML	Cyclohexane	0.0422	0.0314	0.0747	0.0922	0.0787	0.0752	0.0707	0.0745	0.0721		0.07	28	TM	1.000	
44	TM	1,1-Dichloropropene	0.1208	0.1511	0.1539	0.1428	0.1389	0.1433	0.1426	0.1411	0.1399		0.14	6.6	TM		
45	TM	2,2,4-Trimethylpentane	0.1931	0.1842	0.2146	0.2041	0.1754	0.2057	0.1953	0.2074	0.2036		0.20	6.2	TM		
46	S	1,2-DCA-D4(S)	0.2439	0.2350	0.2142	0.2237	0.2148	0.2214	0.2104	0.2099	0.1865		0.22	7.5	S		
47	TM	Carbon Tetrachloride	0.2404	0.2462	0.2756	0.2417	0.2607	0.2647	0.2547	0.2618	0.2525		0.26	4.5	TM		
48	TM	Tert Amyl Methyl Ether	0.2588	0.3044	0.3214	0.3203	0.2968	0.2853	0.2718	0.2748	0.2590		0.29	8.4	TM		
49	TM	1,2-DCA	0.2250	0.2625	0.2525	0.2277	0.2375	0.2346	0.2248	0.2282	0.2153		0.23	6.3	TM		
50	TM	Benzene	0.4155	0.4052	0.4263	0.4229	0.4066	0.3985	0.3965	0.4011	0.3788		0.41	3.6	TM		
51	TM	TCE	0.1196	0.1463	0.1344	0.1261	0.1283	0.1333	0.1264	0.1321	0.1237		0.13	6.0	TM		
52	TM	2-Pentanone	0.0544	0.0541	0.0521	0.0552	0.0519	0.0516	0.0518	0.0549	0.0537		0.05	2.7	TM		
53	TM*	1,2-Dichloropropane	0.0646	0.0493	0.0479	0.0502	0.0481	0.0458	0.0418	0.0447	0.0434		0.05	14	TM*		
54	TM	Bromodichloromethane	0.1351	0.1610	0.2137	0.1959	0.2078	0.2056	0.1973	0.2009	0.1961		0.19	13	TM		
55	TM	Methyl Cyclohexane	0.1287	0.1186	0.1553	0.1577	0.1445	0.1613	0.1467	0.1565	0.1498		0.15	9.7	TM		
56	TM	Dibromomethane	0.0723	0.0828	0.0897	0.0781	0.0820	0.0819	0.0716	0.0750	0.0723		0.08	7.9	TM		
57	TM	MIBK (methyl isobutyl ketone)	0.0660	0.0582	0.0671	0.0680	0.0642	0.0690	0.0649	0.0693	0.0693		0.07	5.4	TM		
58	TML	1-Bromo-2-chloroethane		0.0065	0.0233	0.0322	0.0298	0.0275	0.0278	0.0273	0.0269		0.03	32	TM	1.000	
59	TML	2-Chloroethyl vinyl ether													TM		
60	TM	Cis-1,3-Dichloropropene	0.1980	0.1887	0.1633	0.1710	0.1625	0.1742	0.1738	0.1828	0.1772		0.18	6.5	TM		
61	TM*	Toluene	0.5749	0.5567	0.4775	0.5016	0.4631	0.5035	0.4694	0.4882	0.4758		0.50	7.8	TM*		
62	TM	Trans-1,3-Dichloropropene	0.1596	0.1327	0.1788	0.1736	0.1823	0.1700	0.1649	0.1847	0.1771		0.17	9.4	TM		
63	TM	1,1,2-TCA		0.0896	0.0629	0.0869	0.0687	0.0730	0.0655	0.0733	0.0693		0.07	13	TM		
64	TM	2-Hexanone	0.0357	0.0425	0.0445	0.0450	0.0421	0.0432	0.0428	0.0454	0.0469		0.04	7.4	TM		
65	I	Chlorobenzene-D5 (IS)															
66	S	Toluene-D8(S)	1.358	1.333	1.155	1.159	1.169	1.191	1.151	1.129	1.046		1.2	8.3	S		
67	TM	1,2-EDB	0.0748	0.1296	0.1200	0.1325	0.1308	0.1300	0.1206	0.1181	0.1205		0.12	15	TM		
68	TML	Tetrachloroethene	0.1994	0.1512	0.1208	0.1569	0.1091	0.1202	0.1125	0.1127	0.1090		0.13	23	TM	1.000	
69	TM	1-Chlorohexane	0.1109	0.1026	0.1040	0.0880	0.0946	0.0910	0.0930	0.0954	0.0994		0.10	7.4	TM		
70	TM	1,1,1,2-Tetrachloroethane	0.1918	0.2138	0.2156	0.2158	0.1934	0.1985	0.1898	0.1925	0.1915		0.20	5.7	TM		

VOLATILE ORGANIC ANALYSIS BY  
EPA METHOD 8260B

Form 6  
Initial Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Initial Cal. Date: 11/11/2021  
Instrument: Max

Initials: PA

		Compound	1	2	3	4	5	6	7	8	9		Avg	%RSD	Type	Q	MRF
71	TM	m&p-Xylene	0.2194	0.2838	0.2732	0.2817	0.2638	0.2812	0.2769	0.2781	0.2798		0.27	7.5	TM		
72	TM	o-Xylene	0.2136	0.2399	0.2299	0.2578	0.2962	0.2847	0.2785	0.2733	0.2854		0.26	11	TM		
73	TM	Styrene	0.2970	0.4081	0.4153	0.3968	0.4218	0.4267	0.4487	0.4497	0.4664		0.41	12	TM		
74	S	4-Bromofluorobenzene(S)	0.4452	0.4591	0.4255	0.4207	0.4671	0.4735	0.4671	0.4590	0.4598		0.45	4.1	S		
75	TML	1,3-Dichloropropane	0.0982	0.1309	0.1635	0.1953	0.1861	0.1890	0.1684	0.1806	0.1719		0.16	19	TM	1.000	
76	TM	Dibromochloromethane	0.1814	0.1823	0.1887	0.2191	0.2034	0.1814	0.1871	0.1988	0.1902		0.19	6.5	TM		
77	TM**	Chlorobenzene	0.3488	0.3514	0.4215	0.4387	0.4138	0.4213	0.4007	0.4244	0.4102		0.40	7.9	TM**		
78	TM*	Ethylbenzene	0.4987	0.5093	0.6980	0.6479	0.6576	0.6611	0.6518	0.6525	0.6613		0.63	11	TM*		
79	TM**	Bromoform	0.1375	0.1526	0.1306	0.1492	0.1632	0.1534	0.1524	0.1550	0.1588		0.15	6.8	TM**		
80	I	1,4-Dichlorobenzene-D (IS)															
81	TM	Isopropylbenzene	0.8094	1.001	1.129	1.143	1.116	1.143	1.055	1.121	1.072		1.1	10	TM		
82	TM**	1,1,2,2-Tetrachloroethane	0.1686	0.1692	0.1875	0.2012	0.1859	0.1819	0.1662	0.1664	0.1703		0.18	6.9	TM**		
83	TML	1,2,3-Trichloropropane		0.1292	0.0983	0.1261	0.0934	0.0996	0.0850	0.0886	0.0885		0.10	17	TM	1.000	
84	TML	t-1,4-Dichloro-2-Butene	0.0293	0.0253	0.0636	0.0419	0.0432	0.0426	0.0419	0.0412	0.0441		0.04	26	TM	0.999	
85	TM	Bromobenzene	0.3142	0.4130	0.4968	0.3752	0.3724	0.3835	0.3469	0.3688	0.3576		0.38	13	TM		
86	TM	n-Propylbenzene	0.7774	1.036	0.9314	1.125	1.104	1.114	1.065	1.129	1.097		1.0	11	TM		
87	TM	4-Ethyltoluene	0.9639	0.9886	1.020	1.014	1.036	1.047	1.008	1.070	1.042		1.0	3.2	TM		
88	TM	2-Chlorotoluene	0.6111	0.8380	0.8467	0.8664	0.8837	0.8494	0.8141	0.8418	0.8342		0.82	9.9	TM		
89	TM	1,3,5-Trimethylbenzene	0.6787	0.8751	0.8634	0.9397	0.9607	0.9580	0.9242	0.9630	0.9420		0.90	10	TM		
90	TM	4-Chlorotoluene	0.6712	0.8978	0.8299	0.8338	0.8460	0.8551	0.8384	0.8571	0.8331		0.83	7.6	TM		
91	TM	Tert-Butylbenzene	0.4675	0.3609	0.4687	0.5846	0.5401	0.5532	0.5773	0.5858	0.5880		0.53	15	TM		
92	TM	1,2,4-Trimethylbenzene	0.8328	0.7967	0.7930	0.8177	0.9128	0.9370	0.9311	0.9628	0.9721		0.88	8.3	TM		
93	TM	Sec-Butylbenzene	0.6759	0.9035	0.8662	0.9605	1.032	1.076	1.037	1.110	1.118		0.98	15	TM		
94	TML	p-Isopropyltoluene	0.6771	0.7080	0.8351	0.8201	0.8933	1.014	0.9987	1.079	1.099		0.90	17	TM	1.000	
95	TML	Benzyl Chloride		0.2763	0.2611	0.2465	0.2372	0.2171	0.2142	0.2285	0.2635		0.24	9.3	TM	0.996	
96	TM	1,3-DCB	0.5823	0.6711	0.7030	0.6502	0.7011	0.6493	0.6208	0.6456	0.6458		0.65	5.8	TM		
97	TM	1,4-DCB	0.7778	0.7271	0.6735	0.7099	0.6664	0.6450	0.6210	0.6272	0.6347		0.68	7.8	TM		
98	TML	n-Butylbenzene	0.4730	0.4764	0.4179	0.4761	0.5286	0.5812	0.6108	0.6923	0.7470		0.56	20	TM	0.998	
99	TM	1,2-DCB	0.5592	0.6174	0.5180	0.5611	0.6437	0.6394	0.6237	0.6358	0.6502		0.61	7.8	TM		
100	TML	Hexachloroethane	0.0960	0.1642	0.1790	0.1657	0.1661	0.1696	0.1625	0.1833	0.1868		0.16	16	TM	0.999	
101	TML	1,2-Dibromo-3-chloropropane	0.0273	0.0347	0.0464	0.0354	0.0506	0.0435	0.0499	0.0487	0.0550		0.04	21	TM	0.998	
102	TML	1,2,4-Trichlorobenzene	0.0761	0.1191	0.1424	0.1585	0.1625	0.1957	0.2155	0.2697	0.3199		0.18	41	TM	0.994	
103	TML	Hexachlorobutadiene	0.1600	0.1232	0.1551	0.2151	0.2205	0.2503	0.2545	0.2946	0.3077		0.22	29	TM	0.999	
104	TML	Naphthalene		0.1205	0.2092	0.2187	0.2756	0.3271	0.4007	0.5171	0.6555		0.34	52	TM	0.990	
105	TML	1,2,3-Trichlorobenzene	0.1210	0.1524	0.1497	0.1549	0.1981	0.2341	0.2765	0.3398	0.4162		0.23	44	TM	0.992	

Data File : M:\MAX\DATA\211111\1111M22.D  
 Acq On : 11 Nov 21 18:38  
 Sample : 0.3ug/L VOC STD 11/11/21  
 Misc : IS&S 8/4/21

Vial: 2  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 12 9:06 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:05:35 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.37	96	412529	25.00	ppb	0.00
65) Chlorobenzene-D5 (IS)	9.53	117	369810	25.00	ppb	0.00
80) 1,4-Dichlorobenzene-D (IS)	11.85	152	213533	25.00	ppb	0.00
<b>System Monitoring Compounds</b>						
41) Dibromofluoromethane(S)	5.60	111	28282	5.52	ppb	0.00
Spiked Amount	25.000		Recovery	=	22.080%	
46) 1,2-DCA-D4(S)	5.98	65	20120	5.60	ppb	0.00
Spiked Amount	25.000		Recovery	=	22.388%	
66) Toluene-D8(S)	8.08	98	100459	5.88	ppb	0.00
Spiked Amount	25.000		Recovery	=	23.504%	
74) 4-Bromofluorobenzene(S)	10.70	95	32929	4.78	ppb	0.00
Spiked Amount	25.000		Recovery	=	19.132%	
<b>Target Compounds</b>						
2) Chlorotrifluoroethene	1.04	116	1848	21.79	ppb	# 62
3) Dichlorodifluoromethane	1.20	85	783	0.31	ppb	# 74
4) Freon 114	1.29	85	291	0.20	ppb	# 34
5) Chloromethane	1.34	50	555	0.38	ppb	# 41
6) Vinyl chloride	1.43	62	150	0.08	ppb	# 33
7) 2-Chloro-1,1,1-trifluoroet	1.04	118	1940	40.09	ppb	# 67
8) Bromomethane	1.70	94	576	0.37	ppb	# 96
9) Chloroethane	1.80	64	761	1.81	ppb	# 38
10) Dichlorofluoromethane	1.98	67	979	0.25	ppb	# 42
11) Trichlorofluoromethane	2.03	101	863	0.18	ppb	# 94
12) 2,2-Dichloro-1,1,1-trifluo	2.54	85	170	35.48	ppb	# 100
13) Acrolein	2.45	56	2089	0.61	ppb	# 72
14) Acetone	2.64	43	2754	5.16	ppb	# 99
15) Freon-113	2.54	151	398	0.20	ppb	# 59
16) Acetonitrile	2.95	41	1439	11.22	ppb	# 73
17) 2-propanol	2.29	45	34	2.00	ppb	# 61
18) 1,2-Dichlorotrifluoroethan	1.98	67	979	0.25	ppb	# 100
19) 1,1-DCE	2.53	61	487	0.17	ppb	# 76
20) t-Butanol	3.38	59	1936	13.47	ppb	# 68
21) Methyl Acetate	3.01	43	245	0.27	ppb	# 49
22) Iodomethane	2.69	142	319	1.34	ppb	# 32
25) Methylene chloride	3.10	84	471	0.26	ppb	# 76
26) Carbon disulfide	2.74	76	579	0.25	ppb	# 59
27) Methyl t-butyl ether (MtBE)	3.51	73	918	0.15	ppb	# 97
28) Trans-1,2-DCE	3.46	96	395	0.20	ppb	# 64
31) Diisopropyl Ether	4.29	45	871	0.23	ppb	# 72
32) 1,1-DCA	4.09	63	720	0.24	ppb	# 79

(#) = qualifier out of range (m) = manual integration  
 1111M22.D M1111W.M Fri Nov 12 2021 9:46:14

Quantitation Report (Not Reviewed)

Data File : M:\MAX\DATA\211111\1111M22.D  
 Acq On : 11 Nov 21 18:38  
 Sample : 0.3ug/L VOC STD 11/11/21  
 Misc : IS&S 8/4/21

Vial: 2  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 12 9:06 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:05:35 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
34) Ethyl tert Butyl Ether	4.81	59	1369	0.28	ppb	# 79
35) Methylcyclopentane	4.80	56	78	-1.09	ppb	100
36) MEK (2-Butanone)	5.03	43	3171	5.73	ppb	# 94
37) Cis-1,2-DCE	4.95	96	282	0.13	ppb	# 51
38) 2,2-Dichloropropane	4.94	77	858	0.22	ppb	# 62
39) Chloroform	5.39	83	945	0.24	ppb	# 73
40) Bromochloromethane	5.24	130	303	-0.27	ppb	# 52
42) 1,1,1-TCA	5.58	97	735	0.16	ppb	# 54
43) Cyclohexane	5.62	41	209	0.16	ppb	# 49
44) 1,1-Dichloropropene	5.78	75	598	0.24	ppb	# 75
45) 2,2,4-Trimethylpentane	6.14	57	956	0.29	ppb	90
47) Carbon Tetrachloride	5.76	117	1190	0.27	ppb	# 74
48) Tert Amyl Methyl Ether	6.22	73	1281	0.26	ppb	# 76
49) 1,2-DCA	6.07	62	1114	0.29	ppb	# 26
50) Benzene	6.03	78	2057	0.29	ppb	98
51) TCE	6.79	95	592	0.26	ppb	# 32
52) 2-Pentanone	7.04	43	8982	9.67	ppb	97
53) 1,2-Dichloropropane	7.04	63	320	0.22	ppb	# 77
54) Bromodichloromethane	7.34	83	669	0.21	ppb	78
55) Methyl Cyclohexane	6.96	83	637	0.18	ppb	96
56) Dibromomethane	7.16	93	358	0.25	ppb	# 31
57) MIBK (methyl isobutyl ket	8.01	43	5443	4.57	ppb	# 93
58) 1-Bromo-2-chloroethane	7.47	144	120	0.26	ppb	# 7
59) 2-Chloroethyl vinyl ether	7.70	43	59	76.33	ppb	# 64
60) Cis-1,3-Dichloropropene	7.82	75	980	0.34	ppb	# 43
61) Toluene	8.14	91	2846	0.34	ppb	# 73
62) Trans-1,3-Dichloropropene	8.40	75	790	0.28	ppb	# 41
63) 1,1,2-TCA	8.59	83	195	0.15	ppb	# 23
64) 2-Hexanone	8.86	43	2942	3.70	ppb	# 87
67) 1,2-EDB	9.06	107	332	0.17	ppb	# 72
68) Tetrachloroethene	8.69	164	885	-0.97	ppb	# 72
69) 1-Chlorohexane	9.56	91	492	0.33	ppb	# 67
70) 1,1,1,2-Tetrachloroethane	9.64	131	851	0.31	ppb	# 42
71) m&p-Xylene	9.79	106	1947	0.47	ppb	99
72) o-Xylene	10.19	106	948	0.22	ppb	98
73) Styrene	10.21	104	1318	0.20	ppb	# 87
75) 1,3-Dichloropropane	8.74	76	436	0.15	ppb	# 45
76) Dibromochloromethane	8.95	129	805	0.28	ppb	# 69
77) Chlorobenzene	9.55	112	1548	0.24	ppb	# 57
78) Ethylbenzene	9.67	91	2213	0.22	ppb	# 80
79) Bromoform	10.37	173	610	0.26	ppb	# 73
81) Isopropylbenzene	10.56	105	2074	0.21	ppb	91

(#) = qualifier out of range (m) = manual integration

Quantitation Report (Not Reviewed)

Data File : M:\MAX\DATA\211111\1111M22.D  
 Acq On : 11 Nov 21 18:38  
 Sample : 0.3ug/L VOC STD 11/11/21  
 Misc : IS&S 8/4/21

Vial: 2  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 12 9:06 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:05:35 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
82) 1,1,2,2-Tetrachloroethane	10.87	83	432	0.25	ppb	# 61
83) 1,2,3-Trichloropropane	10.91	110	150	0.17	ppb	84
84) t-1,4-Dichloro-2-Butene	10.92	53	75	0.57	ppb	# 17
85) Bromobenzene	10.84	156	805	0.25	ppb	# 65
86) n-Propylbenzene	10.97	91	1992	0.20	ppb	98
87) 4-Ethyltoluene	11.09	105	2470	0.27	ppb	84
88) 2-Chlorotoluene	11.05	91	1566	0.20	ppb	# 76
89) 1,3,5-Trimethylbenzene	11.14	105	1739	0.21	ppb	93
90) 4-Chlorotoluene	11.15	91	1720	0.22	ppb	# 64
91) Tert-Butylbenzene	11.47	119	1198	0.26	ppb	# 70
92) 1,2,4-Trimethylbenzene	11.51	105	2134	0.27	ppb	83
93) Sec-Butylbenzene	11.69	105	1732	0.19	ppb	# 75
94) p-Isopropyltoluene	11.84	119	1735	0.20	ppb	# 82
95) Benzyl Chloride	12.02	91	644	0.31	ppb	# 75
96) 1,3-DCB	11.78	146	1492	0.26	ppb	91
97) 1,4-DCB	11.88	146	1993	0.35	ppb	92
98) n-Butylbenzene	12.24	91	1212	1.52	ppb	# 75
99) 1,2-DCB	12.24	146	1433	0.26	ppb	# 83
100) Hexachloroethane	12.48	117	246	0.17	ppb	# 17
101) 1,2-Dibromo-3-chloropropan	13.01	75	70	1.41	ppb	# 31
102) 1,2,4-Trichlorobenzene	13.84	180	195	2.28	ppb	# 74
103) Hexachlorobutadiene	14.02	225	410	1.17	ppb	# 46
104) Naphthalene	14.07	128	670	1.33	ppb	# 69
105) 1,2,3-Trichlorobenzene	14.32	180	310	2.72	ppb	# 77



Quantitation Report


Data File : M:\MAX\DATA\211111\1111M22.D  
Acq On : 11 Nov 21 18:38  
Sample : 0.3ug/L VOC STD 11/11/21  
Misc : IS&S 8/4/21

Vial: 2  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Nov 12 9:06 2021

Quant Results File: M1111W.RES

Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Fri Nov 12 09:40:33 2021  
Response via : Initial Calibration



Data File : M:\MAX\DATA\211111\1111M23.D  
 Acq On : 11 Nov 21 19:07  
 Sample : 0.5ug/L VOC STD 11/11/21  
 Misc : IS&S 8/4/21

Vial: 3  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 12 9:06 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:05:35 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.37	96	412615	25.00	ppb	0.00
65) Chlorobenzene-D5 (IS)	9.53	117	365084	25.00	ppb	0.00
80) 1,4-Dichlorobenzene-D (IS)	11.85	152	207406	25.00	ppb	0.00
System Monitoring Compounds						
41) Dibromofluoromethane(S)	5.60	111	27541	5.37	ppb	0.00
Spiked Amount	25.000		Recovery	=	21.496%	
46) 1,2-DCA-D4(S)	5.98	65	19392	5.39	ppb	0.00
Spiked Amount	25.000		Recovery	=	21.572%	
66) Toluene-D8(S)	8.08	98	97321	5.77	ppb	0.00
Spiked Amount	25.000		Recovery	=	23.068%	
74) 4-Bromofluorobenzene(S)	10.70	95	33524	4.93	ppb	0.00
Spiked Amount	25.000		Recovery	=	19.732%	
Target Compounds						
2) Chlorotrifluoroethene	1.02	116	1891	22.29	ppb	# 41
3) Dichlorodifluoromethane	1.20	85	877	0.35	ppb	# 58
4) Freon 114	1.30	85	757	0.53	ppb	# 91
5) Chloromethane	1.34	50	930	0.64	ppb	# 65
6) Vinyl chloride	1.43	62	860	0.49	ppb	# 78
7) 2-Chloro-1,1,1-trifluoroet	1.01	118	2584	53.38	ppb	# 53
8) Bromomethane	1.69	94	1064	0.68	ppb	# 66
9) Chloroethane	1.80	64	925	1.93	ppb	# 38
10) Dichlorofluoromethane	1.99	67	1582	0.40	ppb	# 97
11) Trichlorofluoromethane	2.02	101	2075	0.43	ppb	# 41
12) 2,2-Dichloro-1,1,1-trifluo	2.54	85	369	76.99	ppb	100
13) Acrolein	2.46	56	4660	16.10	ppb	# 81
14) Acetone	2.64	43	5053	9.46	ppb	# 96
15) Freon-113	2.54	151	848	0.43	ppb	# 79
16) Acetonitrile	2.95	41	2898	22.58	ppb	# 86
17) 2-propanol	2.22	45	19	1.12	ppb	# 61
18) 1,2-Dichlorotrifluoroethan	1.99	67	1582	0.40	ppb	100
19) 1,1-DCE	2.54	61	1061	0.37	ppb	# 59
20) t-Butanol	3.37	59	3909	24.10	ppb	# 76
21) Methyl Acetate	3.03	43	477	0.53	ppb	# 85
22) Iodomethane	2.68	142	663	1.49	ppb	# 87
23) Acrylonitrile	3.51	53	121	0.27	ppb	# 18
25) Methylene chloride	3.12	84	483	0.26	ppb	# 74
26) Carbon disulfide	2.74	76	1064	0.46	ppb	# 67
27) Methyl t-butyl ether (MtBE)	3.50	73	3159	0.51	ppb	# 70
28) Trans-1,2-DCE	3.47	96	965	0.48	ppb	# 25
29) 3-Methylpentane	3.50	57	511	0.14	ppb	# 38

(#) = qualifier out of range (m) = manual integration  
 1111M23.D M1111W.M Fri Nov 12 09:46:16 2021

Data File : M:\MAX\DATA\211111\1111M23.D  
 Acq On : 11 Nov 21 19:07  
 Sample : 0.5ug/L VOC STD 11/11/21  
 Misc : IS&S 8/4/21

Vial: 3  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 12 9:06 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:05:35 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
30) Hexane	3.68	56	49	4.71	ppb	100
31) Diisopropyl Ether	4.29	45	1148	0.30	ppb #	85
32) 1,1-DCA	4.10	63	1182	0.39	ppb #	59
34) Ethyl tert Butyl Ether	4.80	59	2386	0.48	ppb #	75
35) Methylcyclopentane	4.83	56	20	-1.40	ppb	100
36) MEK (2-Butanone)	5.03	43	5137	9.28	ppb #	82
37) Cis-1,2-DCE	4.96	96	941	0.43	ppb #	48
38) 2,2-Dichloropropane	4.93	77	2062	0.53	ppb	99
39) Chloroform	5.39	83	2239	0.58	ppb	94
40) Bromochloromethane	5.25	130	943	0.11	ppb	92
42) 1,1,1-TCA	5.58	97	2407	0.52	ppb #	85
43) Cyclohexane	5.61	41	259	0.20	ppb #	47
44) 1,1-Dichloropropene	5.79	75	1247	0.50	ppb	81
45) 2,2,4-Trimethylpentane	6.14	57	1520	0.46	ppb #	42
47) Carbon Tetrachloride	5.78	117	2032	0.47	ppb #	66
48) Tert Amyl Methyl Ether	6.22	73	2512	0.52	ppb #	94
49) 1,2-DCA	6.07	62	2166	0.56	ppb #	78
50) Benzene	6.03	78	3344	0.47	ppb #	84
51) TCE	6.78	95	1207	0.53	ppb #	57
52) 2-Pentanone	7.04	43	22307	24.00	ppb	85
53) 1,2-Dichloropropane	7.03	63	407	0.33	ppb #	77
54) Bromodichloromethane	7.34	83	1329	0.41	ppb #	62
55) Methyl Cyclohexane	6.97	83	979	0.32	ppb #	45
56) Dibromomethane	7.15	93	683	0.49	ppb	78
57) MIBK (methyl isobutyl ket	8.01	43	9605	8.06	ppb	96
58) 1-Bromo-2-chloroethane	7.65	144	54	0.12	ppb #	63
59) 2-Chloroethyl vinyl ether	7.75	43	26	33.63	ppb #	32
60) Cis-1,3-Dichloropropene	7.81	75	1557	0.54	ppb #	70
61) Toluene	8.15	91	4594	0.55	ppb	96
62) Trans-1,3-Dichloropropene	8.40	75	1095	0.38	ppb #	75
63) 1,1,2-TCA	8.58	83	739	0.58	ppb #	54
64) 2-Hexanone	8.86	43	7020	8.82	ppb #	88
67) 1,2-EDB	9.05	107	946	0.49	ppb	85
68) Tetrachloroethene	8.69	164	1104	-0.83	ppb #	72
69) 1-Chlorohexane	9.57	91	749	0.52	ppb #	72
70) 1,1,1,2-Tetrachloroethane	9.65	131	1561	0.58	ppb	82
71) m&p-Xylene	9.80	106	4145	1.01	ppb	78
72) o-Xylene	10.19	106	1752	0.41	ppb	92
73) Styrene	10.20	104	2980	0.46	ppb #	92
75) 1,3-Dichloropropane	8.75	76	956	0.34	ppb #	43
76) Dibromochloromethane	8.96	129	1331	0.47	ppb	86
77) Chlorobenzene	9.56	112	2566	0.41	ppb	89

(#) = qualifier out of range (m) = manual integration  
 1111M23.D M1111W.M Fri Nov 12 09:46:16 2021

Quantitation Report (Not Reviewed)

Data File : M:\MAX\DATA\211111\1111M23.D  
 Acq On : 11 Nov 21 19:07  
 Sample : 0.5ug/L VOC STD 11/11/21  
 Misc : IS&S 8/4/21

Vial: 3  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 12 9:06 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:05:35 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
78) Ethylbenzene	9.68	91	3719	0.37	ppb	96
79) Bromoform	10.37	173	1114	0.48	ppb #	71
81) Isopropylbenzene	10.56	105	4154	0.43	ppb	98
82) 1,1,2,2-Tetrachloroethane	10.87	83	702	0.43	ppb #	62
83) 1,2,3-Trichloropropane	10.90	110	536	0.64	ppb #	62
84) t-1,4-Dichloro-2-Butene	10.93	53	105	0.64	ppb #	17
85) Bromobenzene	10.84	156	1713	0.54	ppb	93
86) n-Propylbenzene	10.96	91	4299	0.45	ppb	92
87) 4-Ethyltoluene	11.08	105	4101	0.47	ppb	89
88) 2-Chlorotoluene	11.04	91	3476	0.46	ppb	98
89) 1,3,5-Trimethylbenzene	11.14	105	3630	0.44	ppb	87
90) 4-Chlorotoluene	11.15	91	3724	0.50	ppb	99
91) Tert-Butylbenzene	11.47	119	1497	0.33	ppb #	75
92) 1,2,4-Trimethylbenzene	11.51	105	3305	0.42	ppb #	67
93) Sec-Butylbenzene	11.68	105	3748	0.43	ppb	92
94) p-Isopropyltoluene	11.84	119	2937	0.35	ppb #	68
95) Benzyl Chloride	12.03	91	1146	0.57	ppb #	87
96) 1,3-DCB	11.78	146	2784	0.51	ppb	85
97) 1,4-DCB	11.87	146	3016	0.54	ppb	86
98) n-Butylbenzene	12.23	91	1976	1.64	ppb #	83
99) 1,2-DCB	12.24	146	2561	0.48	ppb	88
100) Hexachloroethane	12.48	117	681	0.48	ppb #	46
101) 1,2-Dibromo-3-chloropropan	13.01	75	144	1.55	ppb #	3
102) 1,2,4-Trichlorobenzene	13.84	180	494	2.39	ppb #	87
103) Hexachlorobutadiene	14.01	225	511	1.22	ppb #	81
104) Naphthalene	14.07	128	500	1.30	ppb #	69
105) 1,2,3-Trichlorobenzene	14.31	180	632	2.81	ppb #	33

(#) = qualifier out of range (m) = manual integration

Quantitation Report


Data File : M:\MAX\DATA\211111\1111M23.D  
Acq On : 11 Nov 21 19:07  
Sample : 0.5ug/L VOC STD 11/11/21  
Misc : IS&S 8/4/21

Vial: 3  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Nov 12 9:06 2021

Quant Results File: M1111W.RES

Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Fri Nov 12 09:40:33 2021  
Response via : Initial Calibration



Data File : M:\MAX\DATA\211111\1111M24.D  
 Acq On : 11 Nov 21 19:35  
 Sample : 1ug/L VOC STD 11/11/21  
 Misc : IS&S 8/4/21

Vial: 4  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 12 9:06 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:05:35 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.37	96	406373	25.00	ppb	0.00
65) Chlorobenzene-D5 (IS)	9.53	117	352913	25.00	ppb	0.00
80) 1,4-Dichlorobenzene-D (IS)	11.85	152	215896	25.00	ppb	0.00
System Monitoring Compounds						
41) Dibromofluoromethane(S)	5.59	111	47923	9.49	ppb	0.00
Spiked Amount	25.000		Recovery	=	37.980%	
46) 1,2-DCA-D4(S)	5.98	65	34816	9.83	ppb	0.00
Spiked Amount	25.000		Recovery	=	39.328%	
66) Toluene-D8(S)	8.08	98	162985	9.99	ppb	0.00
Spiked Amount	25.000		Recovery	=	39.960%	
74) 4-Bromofluorobenzene(S)	10.70	95	60071	9.14	ppb	0.00
Spiked Amount	25.000		Recovery	=	36.576%	
Target Compounds						
2) Chlorotrifluoroethene	1.01	116	608	7.28	ppb	# 1
3) Dichlorodifluoromethane	1.20	85	1997	0.81	ppb	90
4) Freon 114	1.30	85	1209	0.86	ppb	# 67
5) Chloromethane	1.34	50	1284	0.89	ppb	# 84
6) Vinyl chloride	1.43	62	1810	1.04	ppb	84
7) 2-Chloro-1,1,1-trifluoroet	1.03	118	1962	41.16	ppb	# 77
8) Bromomethane	1.70	94	1466	0.96	ppb	90
9) Chloroethane	1.81	64	1499	2.38	ppb	# 38
10) Dichlorofluoromethane	1.99	67	3146	0.81	ppb	99
11) Trichlorofluoromethane	2.03	101	4276	0.91	ppb	# 75
12) 2,2-Dichloro-1,1,1-trifluo	2.52	85	20	4.24	ppb	100
13) Acrolein	2.46	56	10065	46.74	ppb	99
14) Acetone	2.63	43	9551	18.16	ppb	# 82
15) Freon-113	2.55	151	2082	1.07	ppb	91
16) Acetonitrile	2.96	41	6029	47.70	ppb	# 77
17) 2-propanol	2.27	45	64	3.82	ppb	# 61
18) 1,2-Dichlorotrifluoroethan	1.99	67	3146	0.81	ppb	100
19) 1,1-DCE	2.53	61	3009	1.06	ppb	97
20) t-Butanol	3.37	59	7572	45.08	ppb	93
21) Methyl Acetate	3.03	43	801	0.90	ppb	# 28
22) Iodomethane	2.68	142	1667	1.94	ppb	# 70
23) Acrylonitrile	3.47	53	413	0.86	ppb	# 88
24) 2-Methylpentane	2.15	71	23	5.15	ppb	# 1
25) Methylene chloride	3.12	84	1073	0.59	ppb	97
26) Carbon disulfide	2.73	76	2173	0.95	ppb	# 91
27) Methyl t-butyl ether (MtBE)	3.50	73	5010	0.82	ppb	# 82
28) Trans-1,2-DCE	3.46	96	1820	0.93	ppb	89

(#) = qualifier out of range (m) = manual integration

Data File : M:\MAX\DATA\211111\1111M24.D  
 Acq On : 11 Nov 21 19:35  
 Sample : 1ug/L VOC STD 11/11/21  
 Misc : IS&S 8/4/21

Vial: 4  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 12 9:06 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:05:35 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
29) 3-Methylpentane	3.37	57	1347	1.00	ppb	# 94
30) Hexane	3.72	56	19	1.85	ppb	100
31) Diisopropyl Ether	4.28	45	3593	0.95	ppb	# 81
32) 1,1-DCA	4.10	63	3273	1.10	ppb	# 91
34) Ethyl tert Butyl Ether	4.81	59	4376	0.90	ppb	# 85
35) Methylcyclopentane	4.80	56	22	-1.39	ppb	100
36) MEK (2-Butanone)	5.03	43	9821	18.01	ppb	# 81
37) Cis-1,2-DCE	4.94	96	2201	1.01	ppb	# 54
38) 2,2-Dichloropropane	4.93	77	4077	1.07	ppb	# 73
39) Chloroform	5.39	83	3836	1.01	ppb	89
40) Bromochloromethane	5.26	130	1678	0.57	ppb	# 81
42) 1,1,1-TCA	5.57	97	4612	1.02	ppb	# 79
43) Cyclohexane	5.62	41	1215	0.93	ppb	84
44) 1,1-Dichloropropene	5.79	75	2501	1.02	ppb	87
45) 2,2,4-Trimethylpentane	6.15	57	3488	1.07	ppb	97
47) Carbon Tetrachloride	5.77	117	4480	1.05	ppb	# 76
48) Tert Amyl Methyl Ether	6.22	73	5224	1.09	ppb	97
49) 1,2-DCA	6.07	62	4104	1.08	ppb	# 88
50) Benzene	6.03	78	6930	0.98	ppb	94
51) TCE	6.79	95	2184	0.97	ppb	82
52) 2-Pentanone	7.04	43	42374	46.29	ppb	97
53) 1,2-Dichloropropane	7.02	63	779	0.82	ppb	# 70
54) Bromodichloromethane	7.35	83	3474	1.08	ppb	90
55) Methyl Cyclohexane	6.97	83	2524	0.95	ppb	83
56) Dibromomethane	7.15	93	1458	1.05	ppb	# 65
57) MIBK (methyl isobutyl ket	8.01	43	21815	18.59	ppb	95
58) 1-Bromo-2-chloroethane	7.65	144	378	0.84	ppb	79
59) 2-Chloroethyl vinyl ether	7.72	43	79	103.76	ppb	# 69
60) Cis-1,3-Dichloropropene	7.82	75	2654	0.93	ppb	# 90
61) Toluene	8.14	91	7762	0.95	ppb	97
62) Trans-1,3-Dichloropropene	8.40	75	2907	1.03	ppb	100
63) 1,1,2-TCA	8.58	83	1023	0.81	ppb	# 59
64) 2-Hexanone	8.86	43	14462	18.45	ppb	# 88
67) 1,2-EDB	9.06	107	1694	0.91	ppb	92
68) Tetrachloroethene	8.69	164	1705	-0.44	ppb	86
69) 1-Chlorohexane	9.56	91	1468	1.05	ppb	87
70) 1,1,1,2-Tetrachloroethane	9.65	131	3043	1.16	ppb	85
71) m&p-Xylene	9.79	106	7713	1.95	ppb	99
72) o-Xylene	10.19	106	3246	0.78	ppb	81
73) Styrene	10.20	104	5862	0.94	ppb	92
75) 1,3-Dichloropropane	8.74	76	2308	0.84	ppb	93
76) Dibromochloromethane	8.96	129	2664	0.98	ppb	79

Data File : M:\MAX\DATA\211111\1111M24.D  
 Acq On : 11 Nov 21 19:35  
 Sample : 1ug/L VOC STD 11/11/21  
 Misc : IS&S 8/4/21

Vial: 4  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 12 9:06 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:05:35 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
77) Chlorobenzene	9.56	112	5950	0.98	ppb	91
78) Ethylbenzene	9.68	91	9854	1.02	ppb	98
79) Bromoform	10.37	173	1843	0.81	ppb	99
81) Isopropylbenzene	10.56	105	9746	0.97	ppb	94
82) 1,1,2,2-Tetrachloroethane	10.87	83	1619	0.94	ppb #	68
83) 1,2,3-Trichloropropane	10.90	110	849	0.98	ppb	87
84) t-1,4-Dichloro-2-Butene	10.93	53	549	1.62	ppb #	17
85) Bromobenzene	10.84	156	4290	1.29	ppb	97
86) n-Propylbenzene	10.97	91	8043	0.81	ppb	95
87) 4-Ethyltoluene	11.08	105	8805	0.96	ppb	88
88) 2-Chlorotoluene	11.04	91	7312	0.94	ppb	88
89) 1,3,5-Trimethylbenzene	11.15	105	7456	0.88	ppb	98
90) 4-Chlorotoluene	11.15	91	7167	0.92	ppb	97
91) Tert-Butylbenzene	11.47	119	4048	0.86	ppb #	95
92) 1,2,4-Trimethylbenzene	11.52	105	6848	0.85	ppb	96
93) Sec-Butylbenzene	11.68	105	7480	0.83	ppb	87
94) p-Isopropyltoluene	11.84	119	7212	0.83	ppb	97
95) Benzyl Chloride	12.01	91	2255	1.09	ppb #	81
96) 1,3-DCB	11.78	146	6071	1.06	ppb	92
97) 1,4-DCB	11.87	146	5816	1.00	ppb #	80
98) n-Butylbenzene	12.24	91	3609	1.87	ppb	90
99) 1,2-DCB	12.24	146	4473	0.80	ppb #	82
100) Hexachloroethane	12.48	117	1546	1.04	ppb #	64
101) 1,2-Dibromo-3-chloropropan	13.02	75	401	2.01	ppb #	53
102) 1,2,4-Trichlorobenzene	13.84	180	1230	2.63	ppb #	75
103) Hexachlorobutadiene	14.01	225	1339	1.52	ppb	96
104) Naphthalene	14.08	128	1807	1.59	ppb #	69
105) 1,2,3-Trichlorobenzene	14.32	180	1293	2.97	ppb #	70

(#) = qualifier out of range (m) = manual integration




Data File : M:\MAX\DATA\211111\1111M24.D  
 Acq On : 11 Nov 21 19:35  
 Sample : 1ug/L VOC STD 11/11/21  
 Misc : IS&S 8/4/21

Vial: 4  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 12 9:06 2021

Quant Results File: M1111W.RES

Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:40:33 2021  
 Response via : Initial Calibration



Data File : M:\MAX\DATA\211111\1111M25.D  
 Acq On : 11 Nov 21 20:03  
 Sample : 2ug/L VOC STD 11/11/21  
 Misc : IS&S 8/4/21

Vial: 5  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 12 9:06 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:05:35 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.37	96	404400	25.00	ppb	0.00
65) Chlorobenzene-D5 (IS)	9.53	117	350989	25.00	ppb	0.00
80) 1,4-Dichlorobenzene-D (IS)	11.85	152	214879	25.00	ppb	0.00

System Monitoring Compounds

41) Dibromofluoromethane(S)	5.59	111	48309	9.62	ppb	0.00	
Spiked Amount							Recovery = 38.472%
46) 1,2-DCA-D4(S)	5.98	65	36192	10.27	ppb	0.00	
Spiked Amount							Recovery = 41.080%
66) Toluene-D8(S)	8.08	98	162721	10.03	ppb	0.00	
Spiked Amount							Recovery = 40.116%
74) 4-Bromofluorobenzene(S)	10.70	95	59062	9.04	ppb	0.00	
Spiked Amount							Recovery = 36.160%

Target Compounds

	R.T.	QIon	Response	Conc	Units	Qvalue
2) Chlorotrifluoroethene	1.03	116	1701	20.46	ppb	# 3
3) Dichlorodifluoromethane	1.19	85	4858	1.98	ppb	90
4) Freon 114	1.30	85	3508	2.51	ppb	95
5) Chloromethane	1.34	50	3207	2.24	ppb	95
6) Vinyl chloride	1.43	62	2995	1.73	ppb	# 76
7) 2-Chloro-1,1,1-trifluoroet	1.04	118	1073	22.62	ppb	# 38
8) Bromomethane	1.69	94	4025	2.64	ppb	91
9) Chloroethane	1.80	64	3089	3.61	ppb	93
10) Dichlorofluoromethane	1.99	67	6741	1.74	ppb	95
11) Trichlorofluoromethane	2.02	101	9896	2.11	ppb	93
12) 2,2-Dichloro-1,1,1-trifluo	2.56	85	1772	377.21	ppb	100
13) Acrolein	2.45	56	15037	72.33	ppb	# 77
14) Acetone	2.63	43	14092	26.93	ppb	92
15) Freon-113	2.55	151	4376	2.26	ppb	98
16) Acetonitrile	2.96	41	8331	66.24	ppb	89
17) 2-propanol	2.27	45	257	15.42	ppb	# 61
18) 1,2-Dichlorotrifluoroethan	1.99	67	6741	1.74	ppb	100
19) 1,1-DCE	2.53	61	5157	1.83	ppb	# 90
20) t-Butanol	3.37	59	12522	74.70	ppb	# 82
21) Methyl Acetate	3.03	43	1696	1.92	ppb	95
22) Iodomethane	2.69	142	3524	2.77	ppb	82
23) Acrylonitrile	3.47	53	926	1.91	ppb	# 91
25) Methylene chloride	3.12	84	3416	1.89	ppb	# 75
26) Carbon disulfide	2.74	76	4271	1.87	ppb	99
27) Methyl t-butyl ether (MtBE	3.51	73	11562	1.91	ppb	# 87
28) Trans-1,2-DCE	3.46	96	3131	1.60	ppb	94
29) 3-Methylpentane	3.50	57	1806	1.47	ppb	# 91

(#) = qualifier out of range (m) = manual integration  
 1111M25.D M1111W.M Fri Nov 12 09:46:20 2021

Data File : M:\MAX\DATA\211111\1111M25.D  
 Acq On : 11 Nov 21 20:03  
 Sample : 2ug/L VOC STD 11/11/21  
 Misc : IS&S 8/4/21

Vial: 5  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 12 9:06 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:05:35 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
30) Hexane	3.75	56	46	4.51	ppb	100
31) Diisopropyl Ether	4.28	45	7538	2.00	ppb	95
32) 1,1-DCA	4.10	63	6245	2.11	ppb #	80
34) Ethyl tert Butyl Ether	4.81	59	9864	2.04	ppb	100
35) Methylcyclopentane	4.80	56	421	0.78	ppb #	100
36) MEK (2-Butanone)	5.03	43	16870	31.09	ppb	97
37) Cis-1,2-DCE	4.95	96	4692	2.17	ppb	87
38) 2,2-Dichloropropane	4.94	77	8390	2.21	ppb #	92
39) Chloroform	5.40	83	8432	2.22	ppb #	67
40) Bromochloromethane	5.26	130	3812	1.87	ppb #	80
42) 1,1,1-TCA	5.57	97	9784	2.18	ppb #	90
43) Cyclohexane	5.62	41	2984	2.29	ppb #	49
44) 1,1-Dichloropropene	5.79	75	4619	1.90	ppb	89
45) 2,2,4-Trimethylpentane	6.15	57	6604	2.03	ppb #	53
47) Carbon Tetrachloride	5.77	117	7818	1.84	ppb #	80
48) Tert Amyl Methyl Ether	6.21	73	10362	2.17	ppb #	95
49) 1,2-DCA	6.07	62	7365	1.94	ppb	95
50) Benzene	6.03	78	13682	1.95	ppb	93
51) TCE	6.79	95	4080	1.81	ppb	92
52) 2-Pentanone	7.04	43	66996	73.55	ppb	98
53) 1,2-Dichloropropane	7.02	63	1624	1.93	ppb	99
54) Bromodichloromethane	7.35	83	6339	1.99	ppb	87
55) Methyl Cyclohexane	6.97	83	5101	1.99	ppb	77
56) Dibromomethane	7.15	93	2527	1.83	ppb	91
57) MIBK (methyl isobutyl ket	8.00	43	32993	28.25	ppb	97
58) 1-Bromo-2-chloroethane	7.66	144	1043	2.33	ppb #	61
59) 2-Chloroethyl vinyl ether	7.76	43	47	62.03	ppb #	32
60) Cis-1,3-Dichloropropene	7.82	75	5531	1.95	ppb #	85
61) Toluene	8.14	91	16227	2.00	ppb	91
62) Trans-1,3-Dichloropropene	8.40	75	5617	2.01	ppb	91
63) 1,1,2-TCA	8.58	83	2812	2.24	ppb	93
64) 2-Hexanone	8.86	43	21841	28.00	ppb	96
67) 1,2-EDB	9.06	107	3721	2.01	ppb	99
68) Tetrachloroethene	8.69	164	4406	1.26	ppb #	83
69) 1-Chlorohexane	9.56	91	2470	1.77	ppb #	85
70) 1,1,1,2-Tetrachloroethane	9.65	131	6059	2.33	ppb	84
71) m&p-Xylene	9.80	106	15819	4.01	ppb	84
72) o-Xylene	10.19	106	7240	1.75	ppb	85
73) Styrene	10.20	104	11141	1.80	ppb	92
75) 1,3-Dichloropropane	8.74	76	5483	2.02	ppb	91
76) Dibromochloromethane	8.96	129	6152	2.27	ppb	75
77) Chlorobenzene	9.56	112	12317	2.04	ppb	93

(#) = qualifier out of range (m) = manual integration  
 1111M25.D M1111W.M Fri Nov 12 09:46:21 2021

Data File : M:\MAX\DATA\211111\1111M25.D  
 Acq On : 11 Nov 21 20:03  
 Sample : 2ug/L VOC STD 11/11/21  
 Misc : IS&S 8/4/21

Vial: 5  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 12 9:06 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:05:35 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
78) Ethylbenzene	9.68	91	18193	1.90	ppb	94
79) Bromoform	10.38	173	4190	1.86	ppb	91
81) Isopropylbenzene	10.56	105	19653	1.96	ppb	99
82) 1,1,2,2-Tetrachloroethane	10.87	83	3459	2.03	ppb #	68
83) 1,2,3-Trichloropropane	10.90	110	2168	2.51	ppb	94
84) t-1,4-Dichloro-2-Butene	10.93	53	721	2.01	ppb	86
85) Bromobenzene	10.84	156	6450	1.95	ppb #	58
86) n-Propylbenzene	10.97	91	19340	1.97	ppb	97
87) 4-Ethyltoluene	11.08	105	17429	1.91	ppb	92
88) 2-Chlorotoluene	11.04	91	14893	1.91	ppb	91
89) 1,3,5-Trimethylbenzene	11.14	105	16154	1.91	ppb	83
90) 4-Chlorotoluene	11.15	91	14333	1.85	ppb	95
91) Tert-Butylbenzene	11.46	119	10049	2.14	ppb	93
92) 1,2,4-Trimethylbenzene	11.52	105	14056	1.74	ppb	94
93) Sec-Butylbenzene	11.69	105	16511	1.83	ppb	99
94) p-Isopropyltoluene	11.83	119	14097	1.62	ppb	99
95) Benzyl Chloride	12.01	91	4238	2.05	ppb	90
96) 1,3-DCB	11.78	146	11177	1.96	ppb	88
97) 1,4-DCB	11.87	146	12204	2.10	ppb	92
98) n-Butylbenzene	12.24	91	8185	2.54	ppb	83
99) 1,2-DCB	12.24	146	9645	1.73	ppb #	83
100) Hexachloroethane	12.48	117	2849	1.93	ppb	84
101) 1,2-Dibromo-3-chloropropan	13.01	75	609	2.39	ppb #	75
102) 1,2,4-Trichlorobenzene	13.84	180	2725	3.15	ppb	92
103) Hexachlorobutadiene	14.01	225	3697	2.41	ppb #	71
104) Naphthalene	14.08	128	3760	2.04	ppb #	77
105) 1,2,3-Trichlorobenzene	14.32	180	2662	3.31	ppb	92

(#) = qualifier out of range (m) = manual integration

Quantitation Report


Data File : M:\MAX\DATA\211111\1111M25.D  
Acq On : 11 Nov 21 20:03  
Sample : 2ug/L VOC STD 11/11/21  
Misc : IS&S 8/4/21

Vial: 5  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Nov 12 9:06 2021

Quant Results File: M1111W.RES

Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Fri Nov 12 09:40:33 2021  
Response via : Initial Calibration



Data File : M:\MAX\DATA\211111\1111M26.D  
 Acq On : 11 Nov 21 20:32  
 Sample : 5ug/L VOC STD 11/11/21  
 Misc : IS&S 8/4/21

Vial: 6  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 12 9:06 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:05:35 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.37	96	411540	25.00	ppb	0.00
65) Chlorobenzene-D5 (IS)	9.53	117	360431	25.00	ppb	0.00
80) 1,4-Dichlorobenzene-D (IS)	11.85	152	229293	25.00	ppb	0.00

System Monitoring Compounds

41) Dibromofluoromethane (S)	5.59	111	126663	24.78	ppb	0.00
Spiked Amount	25.000		Recovery	= 99.120%		
46) 1,2-DCA-D4 (S)	5.98	65	88384	24.65	ppb	0.00
Spiked Amount	25.000		Recovery	= 98.584%		
66) Toluene-D8 (S)	8.08	98	421468	25.30	ppb	0.00
Spiked Amount	25.000		Recovery	= 101.184%		
74) 4-Bromofluorobenzene (S)	10.70	95	168355	25.09	ppb	0.00
Spiked Amount	25.000		Recovery	= 100.372%		

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Chlorotrifluoroethene	1.01	116	1153	13.63	ppb	# 76
3) Dichlorodifluoromethane	1.20	85	8691	3.49	ppb	# 80
4) Freon 114	1.30	85	6755	4.75	ppb	94
5) Chloromethane	1.34	50	6022	4.13	ppb	100
6) Vinyl chloride	1.43	62	6859	3.89	ppb	# 78
7) 2-Chloro-1,1,1-trifluoroet	1.03	118	1919	39.75	ppb	# 73
8) Bromomethane	1.69	94	8112	5.22	ppb	97
9) Chloroethane	1.79	64	6137	5.87	ppb	# 81
10) Dichlorofluoromethane	1.99	67	17195	4.36	ppb	91
11) Trichlorofluoromethane	2.02	101	21462	4.50	ppb	94
12) 2,2-Dichloro-1,1,1-trifluo	2.42	85	55	11.50	ppb	100
13) Acrolein	2.46	56	18234	86.10	ppb	96
14) Acetone	2.63	43	18836	35.37	ppb	97
15) Freon-113	2.55	151	10282	5.22	ppb	93
16) Acetonitrile	2.96	41	12079	94.37	ppb	# 85
17) 2-propanol	2.28	45	116	6.84	ppb	# 1
18) 1,2-Dichlorotrifluoroethan	1.99	67	17195	4.36	ppb	# 100
19) 1,1-DCE	2.53	61	11819	4.11	ppb	99
20) t-Butanol	3.37	59	17495	104.12	ppb	# 87
21) Methyl Acetate	3.02	43	4383	4.88	ppb	99
22) Iodomethane	2.68	142	8173	4.78	ppb	97
23) Acrylonitrile	3.47	53	2217	4.44	ppb	# 81
24) 2-Methylpentane	1.97	71	21	4.64	ppb	# 1
25) Methylene chloride	3.12	84	8164	4.44	ppb	93
26) Carbon disulfide	2.74	76	10425	4.50	ppb	98
27) Methyl t-butyl ether (MtBE	3.50	73	29839	4.83	ppb	92
28) Trans-1,2-DCE	3.47	96	8875	4.46	ppb	81

(#) = qualifier out of range (m) = manual integration

Data File : M:\MAX\DATA\211111\1111M26.D  
 Acq On : 11 Nov 21 20:32  
 Sample : 5ug/L VOC STD 11/11/21  
 Misc : IS&S 8/4/21

Vial: 6  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 12 9:06 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:05:35 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
29) 3-Methylpentane	3.50	57	4621	4.27	ppb	95
30) Hexane	3.75	56	92	8.86	ppb	100
31) Diisopropyl Ether	4.28	45	18775	4.90	ppb	91
32) 1,1-DCA	4.10	63	14393	4.78	ppb	93
34) Ethyl tert Butyl Ether	4.81	59	24141	4.90	ppb #	84
35) Methylcyclopentane	4.79	56	1046	4.08	ppb	100
36) MEK (2-Butanone)	5.03	43	21206	38.41	ppb	96
37) Cis-1,2-DCE	4.95	96	10901	4.95	ppb	96
38) 2,2-Dichloropropane	4.93	77	17663	4.57	ppb #	77
39) Chloroform	5.39	83	20966	5.43	ppb	88
40) Bromochloromethane	5.26	130	8759	4.80	ppb	98
42) 1,1,1-TCA	5.57	97	23141	5.06	ppb	97
43) Cyclohexane	5.62	41	6481	4.90	ppb	76
44) 1,1-Dichloropropene	5.78	75	11432	4.62	ppb #	86
45) 2,2,4-Trimethylpentane	6.15	57	14439	4.37	ppb	97
47) Carbon Tetrachloride	5.77	117	21454	4.97	ppb	93
48) Tert Amyl Methyl Ether	6.22	73	24425	5.03	ppb	97
49) 1,2-DCA	6.07	62	19545	5.07	ppb	99
50) Benzene	6.03	78	33463	4.69	ppb	92
51) TCE	6.78	95	10558	4.61	ppb	91
52) 2-Pentanone	7.04	43	85402	92.13	ppb	95
53) 1,2-Dichloropropane	7.02	63	3957	4.89	ppb #	92
54) Bromodichloromethane	7.35	83	17103	5.27	ppb	94
55) Methyl Cyclohexane	6.97	83	11893	4.65	ppb	88
56) Dibromomethane	7.15	93	6753	4.81	ppb	80
57) MIBK (methyl isobutyl ket	8.00	43	42270	35.56	ppb	93
58) 1-Bromo-2-chloroethane	7.65	144	2454	5.40	ppb	75
59) 2-Chloroethyl vinyl ether	7.71	43	24	31.13	ppb #	8
60) Cis-1,3-Dichloropropene	7.82	75	13373	4.63	ppb	88
61) Toluene	8.14	91	38116	4.61	ppb	90
62) Trans-1,3-Dichloropropene	8.40	75	15004	5.27	ppb	94
63) 1,1,2-TCA	8.58	83	5654	4.42	ppb #	77
64) 2-Hexanone	8.85	43	27745	34.95	ppb	97
67) 1,2-EDB	9.06	107	9426	4.95	ppb	85
68) Tetrachloroethene	8.69	164	7864	3.30	ppb	95
69) 1-Chlorohexane	9.56	91	6822	4.76	ppb	94
70) 1,1,1,2-Tetrachloroethane	9.64	131	13944	5.21	ppb	98
71) m&p-Xylene	9.80	106	38029	9.39	ppb	96
72) o-Xylene	10.19	106	21349	5.01	ppb	87
73) Styrene	10.20	104	30408	4.78	ppb	99
75) 1,3-Dichloropropane	8.74	76	13415	4.81	ppb	98
76) Dibromochloromethane	8.96	129	14664	5.27	ppb	98

(#) = qualifier out of range (m) = manual integration

Data File : M:\MAX\DATA\211111\1111M26.D  
 Acq On : 11 Nov 21 20:32  
 Sample : 5ug/L VOC STD 11/11/21  
 Misc : IS&S 8/4/21

Vial: 6  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 12 9:06 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:05:35 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
77) Chlorobenzene	9.56	112	29828	4.80	ppb	92
78) Ethylbenzene	9.68	91	47406	4.81	ppb	98
79) Bromoform	10.37	173	11767	5.09	ppb	89
81) Isopropylbenzene	10.56	105	51163	4.78	ppb	98
82) 1,1,2,2-Tetrachloroethane	10.87	83	8523	4.68	ppb #	82
83) 1,2,3-Trichloropropane	10.90	110	4282	4.64	ppb	88
84) t-1,4-Dichloro-2-Butene	10.93	53	1981	4.53	ppb	86
85) Bromobenzene	10.84	156	17079	4.85	ppb	82
86) n-Propylbenzene	10.97	91	50637	4.82	ppb	99
87) 4-Ethyltoluene	11.08	105	47495	4.89	ppb	93
88) 2-Chlorotoluene	11.04	91	40523	4.88	ppb	97
89) 1,3,5-Trimethylbenzene	11.15	105	44057	4.87	ppb	99
90) 4-Chlorotoluene	11.15	91	38796	4.69	ppb	100
91) Tert-Butylbenzene	11.47	119	24768	4.93	ppb	98
92) 1,2,4-Trimethylbenzene	11.51	105	41861	4.87	ppb	96
93) Sec-Butylbenzene	11.68	105	47327	4.93	ppb	96
94) p-Isopropyltoluene	11.83	119	40964	4.42	ppb	97
95) Benzyl Chloride	12.01	91	10876	4.93	ppb	98
96) 1,3-DCB	11.78	146	32153	5.28	ppb	91
97) 1,4-DCB	11.87	146	30559	4.93	ppb	91
98) n-Butylbenzene	12.24	91	24240	4.68	ppb	92
99) 1,2-DCB	12.24	146	29517	4.96	ppb	92
100) Hexachloroethane	12.48	117	7617	4.84	ppb	81
101) 1,2-Dibromo-3-chloropropan	13.02	75	2319	5.26	ppb	88
102) 1,2,4-Trichlorobenzene	13.83	180	7450	4.61	ppb	91
103) Hexachlorobutadiene	14.01	225	10111	4.58	ppb	88
104) Naphthalene	14.07	128	12639	3.87	ppb	97
105) 1,2,3-Trichlorobenzene	14.32	180	9083	4.78	ppb	96

(#) = qualifier out of range (m) = manual integration.





Data File : M:\MAX\DATA\211111\1111M27.D  
 Acq On : 11 Nov 21 21:00  
 Sample : 10ug/L VOC STD 11/11/21  
 Misc : IS&S 8/4/21

Vial: 7  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 12 9:06 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:05:35 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Internal Standards	R.T.	QI on	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.37	96	400946	25.00	ppb	0.00
65) Chlorobenzene-D5 (IS)	9.53	117	356817	25.00	ppb	0.00
80) 1,4-Dichlorobenzene-D (IS)	11.85	152	231463	25.00	ppb	0.00

#### System Monitoring Compounds

41) Dibromofluoromethane(S)	5.59	111	125593	25.22	ppb	0.00
Spiked Amount			25.000	Recovery =		100.880%
46) 1,2-DCA-D4(S)	5.98	65	88784	25.41	ppb	0.00
Spiked Amount			25.000	Recovery =		101.648%
66) Toluene-D8(S)	8.08	98	424997	25.77	ppb	0.00
Spiked Amount			25.000	Recovery =		103.064%
74) 4-Bromofluorobenzene(S)	10.70	95	168961	25.44	ppb	0.00
Spiked Amount			25.000	Recovery =		101.752%

#### Target Compounds

	R.T.	QI on	Response	Conc	Units	Qvalue
2) Chlorotrifluoroethene	1.01	116	823	9.98	ppb	100
3) Dichlorodifluoromethane	1.20	85	22984	9.46	ppb	100
4) Freon 114	1.30	85	14926	10.78	ppb	100
5) Chloromethane	1.34	50	13183	9.28	ppb	100
6) Vinyl chloride	1.43	62	13203	7.69	ppb	100
7) 2-Chloro-1,1,1-trifluoroet	1.04	118	2348	49.92	ppb	100
8) Bromomethane	1.69	94	15538	10.27	ppb	100
9) Chloroethane	1.79	64	10756	9.58	ppb	100
10) Dichlorofluoromethane	1.99	67	36114	9.39	ppb	100
11) Trichlorofluoromethane	2.02	101	47637	10.24	ppb	100
12) 2,2-Dichloro-1,1,1-trifluo	2.41	85	93	19.97	ppb	100
13) Acrolein	2.46	56	21847	104.83	ppb	100
14) Acetone	2.63	43	23827	45.92	ppb	100
15) Freon-113	2.55	151	20152	10.50	ppb	100
16) Acetonitrile	2.96	41	15121	121.26	ppb	100
17) 2-propanol	2.28	45	825	49.92	ppb	100
18) 1,2-Dichlorotrifluoroethan	1.99	67	36114	9.39	ppb	100
19) 1,1-DCE	2.53	61	26310	9.39	ppb	100
20) t-Butanol	3.37	59	19743	122.14	ppb	100
21) Methyl Acetate	3.02	43	8249	9.43	ppb	100
22) Iodomethane	2.68	142	19181	9.81	ppb	100
23) Acrylonitrile	3.47	53	4623	9.47	ppb	100
24) 2-Methylpentane	2.13	71	44	9.98	ppb	100
25) Methylene chloride	3.11	84	16673	9.30	ppb	100
26) Carbon disulfide	2.74	76	20016	8.86	ppb	100
27) Methyl t-butyl ether (MtBE)	3.50	73	57812	9.61	ppb	100
28) Trans-1,2-DCE	3.47	96	17417	8.98	ppb	100

(#) = qualifier out of range (m) = manual integration

Data File : M:\MAX\DATA\211111\1111M27.D  
 Acq On : 11 Nov 21 21:00  
 Sample : 10ug/L VOC STD 11/11/21  
 Misc : IS&S 8/4/21

Vial: 7  
 Operator: LP, DG, CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 12 9:06 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:05:35 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
29) 3-Methylpentane	3.50	57	9225	9.14	ppb	100
30) Hexane	3.75	56	202	19.97	ppb	100
31) Diisopropyl Ether	4.28	45	36030	9.65	ppb	100
32) 1,1-DCA	4.09	63	29730	10.13	ppb	100
34) Ethyl tert Butyl Ether	4.81	59	45272	9.42	ppb	100
35) Methylcyclopentane	4.80	56	2193	10.51	ppb	100
36) MEK (2-Butanone)	5.02	43	24718	45.95	ppb	100
37) Cis-1,2-DCE	4.95	96	19780	9.22	ppb	100
38) 2,2-Dichloropropane	4.93	77	39032	10.37	ppb	100
39) Chloroform	5.39	83	39076	10.39	ppb	100
40) Bromochloromethane	5.25	130	17072	10.05	ppb	100
42) 1,1,1-TCA	5.57	97	44793	10.05	ppb	100
43) Cyclohexane	5.62	41	12062	9.35	ppb	100
44) 1,1-Dichloropropene	5.79	75	22986	9.53	ppb	100
45) 2,2,4-Trimethylpentane	6.15	57	32996	10.25	ppb	100
47) Carbon Tetrachloride	5.77	117	42451	10.09	ppb	100
48) Tert Amyl Methyl Ether	6.22	73	45755	9.67	ppb	100
49) 1,2-DCA	6.07	62	37625	10.01	ppb	100
50) Benzene	6.03	78	63911	9.20	ppb	100
51) TCE	6.78	95	21382	9.58	ppb	100
52) 2-Pentanone	7.04	43	103468	114.57	ppb	100
53) 1,2-Dichloropropane	7.02	63	7350	9.51	ppb	100
54) Bromodichloromethane	7.34	83	32973	10.43	ppb	100
55) Methyl Cyclohexane	6.97	83	25875	10.47	ppb	100
56) Dibromomethane	7.15	93	13136	9.60	ppb	100
57) MIBK (methyl isobutyl ket	8.00	43	55295	47.75	ppb	100
58) 1-Bromo-2-chloroethane	7.65	144	4417	9.97	ppb	100
59) 2-Chloroethyl vinyl ether	7.71	43	45	59.90	ppb	# 100
60) Cis-1,3-Dichloropropene	7.82	75	27940	9.94	ppb	100
61) Toluene	8.14	91	80753	10.02	ppb	100
62) Trans-1,3-Dichloropropene	8.40	75	27257	9.82	ppb	100
63) 1,1,2-TCA	8.58	83	11706	9.39	ppb	100
64) 2-Hexanone	8.85	43	34667	44.82	ppb	100
67) 1,2-EDB	9.06	107	18555	9.85	ppb	100
68) Tetrachloroethene	8.69	164	17160	9.07	ppb	100
69) 1-Chlorohexane	9.56	91	12989	9.16	ppb	100
70) 1,1,1,2-Tetrachloroethane	9.65	131	28334	10.70	ppb	100
71) m&p-Xylene	9.79	106	80266	20.02	ppb	100
72) o-Xylene	10.19	106	40639	9.64	ppb	100
73) Styrene	10.20	104	60903	9.68	ppb	100
75) 1,3-Dichloropropane	8.74	76	26979	9.77	ppb	100
76) Dibromochloromethane	8.96	129	25889	9.41	ppb	100

(#) = qualifier out of range (m) = manual integration

Data File : M:\MAX\DATA\211111\1111M27.D  
 Acq On : 11 Nov 21 21:00  
 Sample : 10ug/L VOC STD 11/11/21  
 Misc : IS&S 8/4/21

Vial: 7  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 12 9:06 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:05:35 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
77) Chlorobenzene	9.55	112	60128	9.78	ppb	100
78) Ethylbenzene	9.68	91	94352	9.67	ppb	100
79) Bromoform	10.37	173	21895	9.57	ppb	100
81) Isopropylbenzene	10.56	105	105829	9.79	ppb	100
82) 1,1,2,2-Tetrachloroethane	10.87	83	16839	9.16	ppb	100
83) 1,2,3-Trichloropropane	10.90	110	9218	9.91	ppb	100
84) t-1,4-Dichloro-2-Butene	10.92	53	3942	8.55	ppb	100
85) Bromobenzene	10.84	156	35508	9.98	ppb	100
86) n-Propylbenzene	10.97	91	103172	9.74	ppb	100
87) 4-Ethyltoluene	11.08	105	96927	9.88	ppb	100
88) 2-Chlorotoluene	11.04	91	78642	9.39	ppb	100
89) 1,3,5-Trimethylbenzene	11.14	105	88696	9.72	ppb	100
90) 4-Chlorotoluene	11.15	91	79169	9.49	ppb	100
91) Tert-Butylbenzene	11.47	119	51216	10.11	ppb	100
92) 1,2,4-Trimethylbenzene	11.51	105	86750	9.99	ppb	100
93) Sec-Butylbenzene	11.68	105	99580	10.27	ppb	100
94) p-Isopropyltoluene	11.83	119	93919	10.04	ppb	100
95) Benzyl Chloride	12.01	91	20103	9.03	ppb	100
96) 1,3-DCB	11.78	146	60112	9.79	ppb	100
97) 1,4-DCB	11.87	146	59719	9.55	ppb	100
98) n-Butylbenzene	12.24	91	53810	8.69	ppb	100
99) 1,2-DCB	12.24	146	59199	9.86	ppb	100
100) Hexachloroethane	12.48	117	15707	9.89	ppb	100
101) 1,2-Dibromo-3-chloropropan	13.01	75	4028	8.13	ppb	100
102) 1,2,4-Trichlorobenzene	13.84	180	18120	7.99	ppb	100
103) Hexachlorobutadiene	14.01	225	23171	9.10	ppb	100
104) Naphthalene	14.08	128	30282	7.46	ppb	100
105) 1,2,3-Trichlorobenzene	14.32	180	21674	7.70	ppb	100

(#) = qualifier out of range (m) = manual integration  
 1111M27.D M1111W.M Fri Nov 12 09:46:25 2021

Quantitation Report


Data File : M:\MAX\DATA\211111\1111M27.D  
Acq On : 11 Nov 21 21:00  
Sample : 10ug/L VOC STD 11/11/21  
Misc : IS&S 8/4/21

Vial: 7  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Nov 12 9:06 2021

Quant Results File: M1111W.RES

Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Fri Nov 12 09:40:33 2021  
Response via : Initial Calibration



Data File : M:\MAX\DATA\211111\1111M28.D  
 Acq On : 11 Nov 21 21:28  
 Sample : 20ug/L VOC STD 11/11/21  
 Misc : IS&S 8/4/21

Vial: 8  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 12 9:06 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:05:35 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.37	96	404029	25.00	ppb	0.00
65) Chlorobenzene-D5 (IS)	9.53	117	358338	25.00	ppb	0.00
80) 1,4-Dichlorobenzene-D (IS)	11.85	152	243425	25.00	ppb	0.00

System Monitoring Compounds

41) Dibromofluoromethane (S)	5.59	111	252655	50.35	ppb	0.00
Spiked Amount			25.000	Recovery =		201.388%
46) 1,2-DCA-D4 (S)	5.98	65	169984	48.28	ppb	0.00
Spiked Amount			25.000	Recovery =		193.128%
66) Toluene-D8 (S)	8.08	98	825135	49.81	ppb	0.00
Spiked Amount			25.000	Recovery =		199.248%
74) 4-Bromofluorobenzene (S)	10.70	95	334735	50.18	ppb	0.00
Spiked Amount			25.000	Recovery =		200.728%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Chlorotrifluoroethene	1.04	116	1836	22.10	ppb	# 1
3) Dichlorodifluoromethane	1.19	85	44816	18.31	ppb	97
4) Freon 114	1.30	85	29562	21.18	ppb	87
5) Chloromethane	1.34	50	22624	15.81	ppb	98
6) Vinyl chloride	1.43	62	29171	16.86	ppb	# 75
7) 2-Chloro-1,1,1-trifluoroet	1.01	118	1756	37.05	ppb	# 41
8) Bromomethane	1.69	94	30220	19.82	ppb	99
9) Chloroethane	1.78	64	18499	15.49	ppb	96
10) Dichlorofluoromethane	1.99	67	68067	17.56	ppb	99
11) Trichlorofluoromethane	2.02	101	90145	19.24	ppb	98
12) 2,2-Dichloro-1,1,1-trifluo	2.54	85	15422	3285.92	ppb	100
13) Acrolein	2.46	56	27582	128.66	ppb	97
14) Acetone	2.63	43	28929	55.33	ppb	99
15) Freon-113	2.55	151	37628	19.45	ppb	# 81
16) Acetonitrile	2.96	41	17905	142.49	ppb	93
17) 2-propanol	2.28	45	1239	74.40	ppb	# 89
18) 1,2-Dichlorotrifluoroethan	1.99	67	68067	17.56	ppb	100
19) 1,1-DCE	2.53	61	50251	17.80	ppb	99
20) t-Butanol	3.38	59	23857	149.77	ppb	# 81
21) Methyl Acetate	3.02	43	14521	16.47	ppb	87
22) Iodomethane	2.68	142	40884	19.41	ppb	94
23) Acrylonitrile	3.47	53	8995	18.25	ppb	# 91
24) 2-Methylpentane	2.05	71	24	5.40	ppb	# 1
25) Methylene chloride	3.11	84	32606	18.06	ppb	93
26) Carbon disulfide	2.73	76	37720	16.57	ppb	# 93
27) Methyl t-butyl ether (MtBE)	3.50	73	109398	18.05	ppb	97
28) Trans-1,2-DCE	3.46	96	33987	17.39	ppb	97

(#) = qualifier out of range (m) = manual integration

Data File : M:\MAX\DATA\211111\1111M28.D  
 Acq On : 11 Nov 21 21:28  
 Sample : 20ug/L VOC STD 11/11/21  
 Misc : IS&S 8/4/21

Vial: 8  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 12 9:06 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:05:35 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
29) 3-Methylpentane	3.50	57	18284	18.34	ppb	# 97
30) Hexane	3.75	56	116	11.38	ppb	100
31) Diisopropyl Ether	4.28	45	72616	19.31	ppb	95
32) 1,1-DCA	4.09	63	57059	19.29	ppb	96
34) Ethyl tert Butyl Ether	4.80	59	87044	17.98	ppb	100
35) Methylcyclopentane	4.80	56	4177	21.20	ppb	100
36) MEK (2-Butanone)	5.02	43	30148	55.62	ppb	# 87
37) Cis-1,2-DCE	4.95	96	41425	19.16	ppb	94
38) 2,2-Dichloropropane	4.93	77	70981	18.71	ppb	# 89
39) Chloroform	5.39	83	78196	20.63	ppb	94
40) Bromochloromethane	5.25	130	32800	19.56	ppb	90
42) 1,1,1-TCA	5.57	97	90169	20.07	ppb	96
43) Cyclohexane	5.62	41	22845	17.58	ppb	88
44) 1,1-Dichloropropene	5.78	75	46082	18.97	ppb	88
45) 2,2,4-Trimethylpentane	6.15	57	63118	19.47	ppb	95
47) Carbon Tetrachloride	5.77	117	82321	19.42	ppb	87
48) Tert Amyl Methyl Ether	6.21	73	87845	18.43	ppb	94
49) 1,2-DCA	6.07	62	72663	19.19	ppb	97
50) Benzene	6.03	78	128173	18.30	ppb	95
51) TCE	6.78	95	40845	18.17	ppb	97
52) 2-Pentanone	7.03	43	125452	137.85	ppb	99
53) 1,2-Dichloropropane	7.03	63	13498	17.49	ppb	98
54) Bromodichloromethane	7.34	83	63782	20.02	ppb	92
55) Methyl Cyclohexane	6.96	83	47414	19.10	ppb	95
56) Dibromomethane	7.15	93	23136	16.78	ppb	93
57) MIBK (methyl isobutyl ket	8.00	43	62903	53.90	ppb	# 92
58) 1-Bromo-2-chloroethane	7.65	144	8974	20.11	ppb	91
59) 2-Chloroethyl vinyl ether	7.72	43	19	25.10	ppb	# 32
60) Cis-1,3-Dichloropropene	7.82	75	56160	19.82	ppb	95
61) Toluene	8.14	91	151728	18.69	ppb	96
62) Trans-1,3-Dichloropropene	8.40	75	53294	19.05	ppb	93
63) 1,1,2-TCA	8.57	83	21157	16.84	ppb	93
64) 2-Hexanone	8.85	43	41456	53.19	ppb	99
67) 1,2-EDB	9.06	107	34558	18.27	ppb	85
68) Tetrachloroethene	8.69	164	32240	18.27	ppb	96
69) 1-Chlorohexane	9.56	91	26656	18.71	ppb	93
70) 1,1,1,2-Tetrachloroethane	9.65	131	54422	20.46	ppb	94
71) m&p-Xylene	9.79	106	158733	39.43	ppb	97
72) o-Xylene	10.19	106	79841	18.85	ppb	100
73) Styrene	10.20	104	128641	20.36	ppb	99
75) 1,3-Dichloropropane	8.74	76	48269	17.40	ppb	85
76) Dibromochloromethane	8.96	129	53624	19.40	ppb	87

(#) = qualifier out of range (m) = manual integration  
 1111M28.D M1111W.M Fri Nov 12 09:46:27 2021

Data File : M:\MAX\DATA\211111\1111M28.D  
 Acq On : 11 Nov 21 21:28  
 Sample : 20ug/L VOC STD 11/11/21  
 Misc : IS&S 8/4/21

Vial: 8  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 12 9:06 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:05:35 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
77) Chlorobenzene	9.55	112	114870	18.60	ppb	97
78) Ethylbenzene	9.68	91	186863	19.07	ppb	98
79) Bromoform	10.37	173	43702	19.02	ppb	97
81) Isopropylbenzene	10.56	105	205496	18.07	ppb	99
82) 1,1,2,2-Tetrachloroethane	10.87	83	32364	16.74	ppb	93
83) 1,2,3-Trichloropropane	10.90	110	16544	16.90	ppb	99
84) t-1,4-Dichloro-2-Butene	10.93	53	8153	16.42	ppb	96
85) Bromobenzene	10.84	156	67558	18.06	ppb	83
86) n-Propylbenzene	10.97	91	207359	18.61	ppb	97
87) 4-Ethyltoluene	11.08	105	196238	19.02	ppb	98
88) 2-Chlorotoluene	11.04	91	158529	17.99	ppb	100
89) 1,3,5-Trimethylbenzene	11.14	105	179984	18.75	ppb	98
90) 4-Chlorotoluene	11.15	91	163273	18.61	ppb	95
91) Tert-Butylbenzene	11.47	119	112432	21.10	ppb	95
92) 1,2,4-Trimethylbenzene	11.51	105	181331	19.85	ppb	97
93) Sec-Butylbenzene	11.68	105	202000	19.80	ppb	97
94) p-Isopropyltoluene	11.83	119	194486	19.76	ppb	98
95) Benzyl Chloride	12.01	91	41709	17.81	ppb	100
96) 1,3-DCB	11.78	146	120893	18.71	ppb	98
97) 1,4-DCB	11.87	146	120929	18.38	ppb	95
98) n-Butylbenzene	12.24	91	118945	16.80	ppb	96
99) 1,2-DCB	12.24	146	121451	19.23	ppb	96
100) Hexachloroethane	12.48	117	31640	18.94	ppb	89
101) 1,2-Dibromo-3-chloropropan	13.02	75	9721	17.01	ppb	85
102) 1,2,4-Trichlorobenzene	13.84	180	41960	14.94	ppb	96
103) Hexachlorobutadiene	14.01	225	49567	17.46	ppb	93
104) Naphthalene	14.08	128	78035	15.94	ppb	98
105) 1,2,3-Trichlorobenzene	14.32	180	53846	14.58	ppb	94



Quantitation Report


Data File : M:\MAX\DATA\211111\1111M28.D  
Acq On : 11 Nov 21 21:28  
Sample : 20ug/L VOC STD 11/11/21  
Misc : IS&S 8/4/21

Vial: 8  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Nov 12 9:06 2021

Quant Results File: M1111W.RES

Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Fri Nov 12 09:40:33 2021  
Response via : Initial Calibration



Data File : M:\MAX\DATA\211111\1111M29.D  
 Acq On : 11 Nov 21 21:57  
 Sample : 40ug/L VOC STD 11/11/21  
 Misc : IS&S 8/4/21

Vial: 9  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 12 9:06 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:05:35 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.37	96	410532	25.00	ppb	0.00
65) Chlorobenzene-D5 (IS)	9.53	117	372777	25.00	ppb	0.00
80) 1,4-Dichlorobenzene-D (IS)	11.84	152	245394	25.00	ppb	0.00

System Monitoring Compounds

41) Dibromofluoromethane(S)	5.59	111	259251	50.84	ppb	0.00	
Spiked Amount				25.000			Recovery = 203.372%
46) 1,2-DCA-D4(S)	5.98	65	172352	48.18	ppb	0.00	
Spiked Amount				25.000			Recovery = 192.716%
66) Toluene-D8(S)	8.08	98	841773	48.85	ppb	0.00	
Spiked Amount				25.000			Recovery = 195.396%
74) 4-Bromofluorobenzene(S)	10.70	95	342243	49.32	ppb	0.00	
Spiked Amount				25.000			Recovery = 197.280%

Target Compounds

	R.T.	QIon	Response	Conc	Units	Qvalue
2) Chlorotrifluoroethene	1.02	116	1920	22.75	ppb #	85
3) Dichlorodifluoromethane	1.19	85	91848	36.94	ppb	100
4) Freon 114	1.30	85	61558	43.40	ppb	93
5) Chloromethane	1.34	50	52016	35.78	ppb	98
6) Vinyl chloride	1.43	62	58412	33.22	ppb	84
7) 2-Chloro-1,1,1-trifluoroet	1.04	118	2375	49.31	ppb #	28
8) Bromomethane	1.69	94	59595	38.46	ppb	99
9) Chloroethane	1.78	64	37432	29.62	ppb	97
10) Dichlorofluoromethane	1.99	67	145200	36.87	ppb	99
11) Trichlorofluoromethane	2.01	101	188147	39.52	ppb	100
12) 2,2-Dichloro-1,1,1-trifluo	2.55	85	30548	6405.68	ppb	100
13) Acrolein	2.46	56	32594	147.22	ppb	95
14) Acetone	2.63	43	38611	72.68	ppb	98
15) Freon-113	2.55	151	81158	41.29	ppb	90
16) Acetonitrile	2.96	41	21885	171.41	ppb	97
17) 2-propanol	2.29	45	2841	167.89	ppb #	83
18) 1,2-Dichlorotrifluoroethan	1.99	67	145200	36.87	ppb	100
19) 1,1-DCE	2.53	61	105741	36.86	ppb	96
20) t-Butanol	3.38	59	35344	237.46	ppb #	80
21) Methyl Acetate	3.02	43	32588	36.34	ppb	97
22) Iodomethane	2.68	142	94938	42.82	ppb	90
23) Acrylonitrile	3.46	53	18608	37.13	ppb #	84
24) 2-Methylpentane	2.11	71	120	26.59	ppb #	1
25) Methylene chloride	3.11	84	66806	36.41	ppb	86
26) Carbon disulfide	2.73	76	82112	35.50	ppb	97
27) Methyl t-butyl ether (MtBE	3.50	73	237272	38.53	ppb	96
28) Trans-1,2-DCE	3.46	96	72259	36.38	ppb	93

(#) = qualifier out of range (m) = manual integration

Data File : M:\MAX\DATA\211111\1111M29.D  
 Acq On : 11 Nov 21 21:57  
 Sample : 40ug/L VOC STD 11/11/21  
 Misc : IS&S 8/4/21

Vial: 9  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 12 9:06 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:05:35 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
29) 3-Methylpentane	3.50	57	39446	39.37	ppb	95
30) Hexane	3.74	56	520	50.20	ppb #	100
31) Diisopropyl Ether	4.28	45	153571	40.19	ppb	97
32) 1,1-DCA	4.09	63	116612	38.79	ppb	95
34) Ethyl tert Butyl Ether	4.80	59	186951	38.00	ppb	97
35) Methylcyclopentane	4.80	56	7494	38.58	ppb	100
36) MEK (2-Butanone)	5.02	43	41437	75.23	ppb	95
37) Cis-1,2-DCE	4.95	96	82080	37.35	ppb	91
38) 2,2-Dichloropropane	4.93	77	148357	38.50	ppb	97
39) Chloroform	5.39	83	163342	42.41	ppb	92
40) Bromochloromethane	5.25	130	65934	39.14	ppb	96
42) 1,1,1-TCA	5.57	97	185118	40.55	ppb	98
43) Cyclohexane	5.62	41	48922	37.05	ppb	87
44) 1,1-Dichloropropene	5.78	75	92663	37.54	ppb	94
45) 2,2,4-Trimethylpentane	6.15	57	136200	41.34	ppb	97
47) Carbon Tetrachloride	5.77	117	171977	39.93	ppb	98
48) Tert Amyl Methyl Ether	6.21	73	180481	37.27	ppb	96
49) 1,2-DCA	6.07	62	149890	38.96	ppb	98
50) Benzene	6.03	78	263460	37.02	ppb	94
51) TCE	6.78	95	86779	37.99	ppb	99
52) 2-Pentanone	7.03	43	157666	170.51	ppb	97
53) 1,2-Dichloropropane	7.02	63	29375	37.67	ppb	97
54) Bromodichloromethane	7.34	83	131973	40.76	ppb	93
55) Methyl Cyclohexane	6.97	83	102821	40.84	ppb	98
56) Dibromomethane	7.15	93	49294	35.19	ppb	91
57) MIBK (methyl isobutyl ket	8.00	43	91035	76.77	ppb	94
58) 1-Bromo-2-chloroethane	7.65	144	17920	39.51	ppb	92
59) 2-Chloroethyl vinyl ether	7.77	43	88	114.41	ppb #	32
60) Cis-1,3-Dichloropropene	7.82	75	120096	41.72	ppb	92
61) Toluene	8.14	91	320702	38.88	ppb	96
62) Trans-1,3-Dichloropropene	8.40	75	121311	42.68	ppb	95
63) 1,1,2-TCA	8.58	83	48125	37.71	ppb	98
64) 2-Hexanone	8.85	43	59620	75.28	ppb	98
67) 1,2-EDB	9.06	107	70434	35.79	ppb #	77
68) Tetrachloroethene	8.69	164	67208	38.12	ppb	97
69) 1-Chlorohexane	9.56	91	56896	38.40	ppb	95
70) 1,1,1,2-Tetrachloroethane	9.65	131	114802	41.48	ppb	99
71) m&p-Xylene	9.80	106	331735	79.22	ppb	100
72) o-Xylene	10.19	106	163008	37.00	ppb	99
73) Styrene	10.20	104	268247	40.81	ppb	97
75) 1,3-Dichloropropane	8.74	76	107722	37.32	ppb	94
76) Dibromochloromethane	8.96	129	118556	41.23	ppb	94

(#) = qualifier out of range (m) = manual integration

1111M29.D M1111W.M Fri Nov 12 09:46:29 2021

Page 2

Data File : M:\MAX\DATA\211111\1111M29.D  
 Acq On : 11 Nov 21 21:57  
 Sample : 40ug/L VOC STD 11/11/21  
 Misc : IS&S 8/4/21

Vial: 9  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 12 9:06 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:05:35 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
77) Chlorobenzene	9.55	112	253152	39.40	ppb	93
78) Ethylbenzene	9.68	91	389158	38.18	ppb	99
79) Bromoform	10.37	173	92475	38.69	ppb	93
81) Isopropylbenzene	10.56	105	440003	38.39	ppb	100
82) 1,1,2,2-Tetrachloroethane	10.87	83	65314	33.51	ppb	# 97
83) 1,2,3-Trichloropropane	10.90	110	34803	35.27	ppb	91
84) t-1,4-Dichloro-2-Butene	10.92	53	16174	31.93	ppb	96
85) Bromobenzene	10.84	156	144813	38.41	ppb	86
86) n-Propylbenzene	10.97	91	443246	39.46	ppb	96
87) 4-Ethyltoluene	11.08	105	420235	40.40	ppb	99
88) 2-Chlorotoluene	11.04	91	330523	37.21	ppb	96
89) 1,3,5-Trimethylbenzene	11.14	105	378109	39.08	ppb	100
90) 4-Chlorotoluene	11.15	91	336524	38.05	ppb	92
91) Tert-Butylbenzene	11.47	119	230016	42.82	ppb	98
92) 1,2,4-Trimethylbenzene	11.51	105	378010	41.05	ppb	100
93) Sec-Butylbenzene	11.68	105	435797	42.38	ppb	99
94) p-Isopropyltoluene	11.83	119	423619	42.70	ppb	97
95) Benzyl Chloride	12.01	91	89732	38.01	ppb	96
96) 1,3-DCB	11.78	146	253470	38.92	ppb	99
97) 1,4-DCB	11.87	146	246246	37.13	ppb	98
98) n-Butylbenzene	12.24	91	271806	36.38	ppb	98
99) 1,2-DCB	12.24	146	249651	39.20	ppb	97
100) Hexachloroethane	12.48	117	71950	42.71	ppb	84
101) 1,2-Dibromo-3-chloropropan	13.01	75	19128	31.99	ppb	95
102) 1,2,4-Trichlorobenzene	13.83	180	105896	34.06	ppb	95
103) Hexachlorobutadiene	14.01	225	115668	39.08	ppb	93
104) Naphthalene	14.08	128	203041	35.98	ppb	98
105) 1,2,3-Trichlorobenzene	14.32	180	133413	31.99	ppb	98

(#) = qualifier out of range (m) = manual integration

1111M29.D M1111W.M

Fri Nov 12 09:46:29 2021

Page 3

Quantitation Report


Data File : M:\MAX\DATA\211111\1111M29.D  
Acq On : 11 Nov 21 21:57  
Sample : 40ug/L VOC STD 11/11/21  
Misc : IS&S 8/4/21

Vial: 9  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Nov 12 9:06 2021

Quant Results File: M1111W.RES

Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Fri Nov 12 09:40:33 2021  
Response via : Initial Calibration



Data File : M:\MAX\DATA\211111\1111M30.D  
 Acq On : 11 Nov 21 22:25  
 Sample : 100ug/L VOC STD 11/11/21  
 Misc : IS&S 8/4/21

Vial: 10  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 12 9:06 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:05:35 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.37	96	401409	25.00	ppb	0.00
65) Chlorobenzene-D5 (IS)	9.53	117	366234	25.00	ppb	0.00
80) 1,4-Dichlorobenzene-D (IS)	11.84	152	257008	25.00	ppb	0.00
System Monitoring Compounds						
41) Dibromofluoromethane(S)	5.59	111	457653	91.79	ppb	0.00
Spiked Amount	25.000		Recovery	=	367.172%	
46) 1,2-DCA-D4(S)	5.98	65	299456	85.61	ppb	0.00
Spiked Amount	25.000		Recovery	=	342.444%	
66) Toluene-D8(S)	8.08	98	1531875	90.48	ppb	0.00
Spiked Amount	25.000		Recovery	=	361.936%	
74) 4-Bromofluorobenzene(S)	10.70	95	673598	98.81	ppb	0.00
Spiked Amount	25.000		Recovery	=	395.224%	
Target Compounds						
2) Chlorotrifluoroethene	1.00	116	147	1.78	ppb	# 44
3) Dichlorodifluoromethane	1.19	85	226688	93.24	ppb	99
4) Freon 114	1.30	85	150805	108.74	ppb	91
5) Chloromethane	1.34	50	124679	87.71	ppb	100
6) Vinyl chloride	1.43	62	142336	82.79	ppb	84
7) 2-Chloro-1,1,1-trifluoroet	1.02	118	2151	45.68	ppb	# 84
8) Bromomethane	1.69	94	142416	94.01	ppb	98
9) Chloroethane	1.77	64	120449	94.64	ppb	90
10) Dichlorofluoromethane	1.98	67	338991	88.03	ppb	98
11) Trichlorofluoromethane	2.00	101	437079	93.89	ppb	97
12) 2,2-Dichloro-1,1,1-trifluo	2.54	85	72338	15513.46	ppb	# 100
13) Acrolein	2.46	56	36951	166.51	ppb	86
14) Acetone	2.64	43	49535	95.36	ppb	97
15) Freon-113	2.54	151	186024	96.80	ppb	86
16) Acetonitrile	2.97	41	25034	200.53	ppb	# 82
17) 2-propanol	2.27	45	125	7.55	ppb	# 61
18) 1,2-Dichlorotrifluoroethan	1.98	67	338991	88.03	ppb	# 100
19) 1,1-DCE	2.52	61	254599	90.78	ppb	98
20) t-Butanol	3.40	59	49220	420.89	ppb	# 91
21) Methyl Acetate	3.02	43	76120	86.64	ppb	91
22) Iodomethane	2.68	142	236547	107.26	ppb	94
23) Acrylonitrile	3.47	53	43725	89.19	ppb	90
24) 2-Methylpentane	2.10	71	723	163.86	ppb	# 7
25) Methylene chloride	3.11	84	160077	89.22	ppb	86
26) Carbon disulfide	2.73	76	179840	79.52	ppb	95
27) Methyl t-butyl ether (MtBE)	3.50	73	525547	87.28	ppb	97
28) Trans-1,2-DCE	3.46	96	167296	86.14	ppb	97

(#) = qualifier out of range (m) = manual integration  
 1111M30.D M1111W.M Fri Nov 12 09:46:31 2021

Data File : M:\MAX\DATA\211111\1111M30.D  
 Acq On : 11 Nov 21 22:25  
 Sample : 100ug/L VOC STD 11/11/21  
 Misc : IS&S 8/4/21

Vial: 10  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 12 9:06 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:05:35 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
29) 3-Methylpentane	3.50	57	87114	89.39	ppb	100
30) Hexane	3.74	56	1307	129.05	ppb #	100
31) Diisopropyl Ether	4.28	45	362535	97.03	ppb	99
32) 1,1-DCA	4.09	63	270425	92.01	ppb	98
34) Ethyl tert Butyl Ether	4.80	59	430166	89.43	ppb	99
35) Methylcyclopentane	4.80	56	16875	90.81	ppb #	100
36) MEK (2-Butanone)	5.03	43	50752	94.24	ppb	95
37) Cis-1,2-DCE	4.94	96	192790	89.73	ppb	92
38) 2,2-Dichloropropane	4.92	77	341813	90.71	ppb	98
39) Chloroform	5.39	83	381193	101.23	ppb	97
40) Bromochloromethane	5.25	130	154971	94.73	ppb	90
42) 1,1,1-TCA	5.57	97	424060	95.00	ppb	97
43) Cyclohexane	5.62	41	115778	89.68	ppb	91
44) 1,1-Dichloropropene	5.78	75	224703	93.09	ppb	92
45) 2,2,4-Trimethylpentane	6.15	57	326876	101.47	ppb	99
47) Carbon Tetrachloride	5.77	117	405417	96.27	ppb	95
48) Tert Amyl Methyl Ether	6.21	73	415894	87.83	ppb #	94
49) 1,2-DCA	6.07	62	345748	91.92	ppb	100
50) Benzene	6.03	78	608246	87.42	ppb	95
51) TCE	6.78	95	198550	88.90	ppb	97
52) 2-Pentanone	7.04	43	172512	190.80	ppb	93
53) 1,2-Dichloropropane	7.02	63	69624	91.60	ppb	99
54) Bromodichloromethane	7.34	83	314864	99.46	ppb	97
55) Methyl Cyclohexane	6.97	83	240488	97.80	ppb	97
56) Dibromomethane	7.15	93	116110	84.78	ppb	93
57) MIBK (methyl isobutyl ket	8.01	43	111277	95.98	ppb	99
58) 1-Bromo-2-chloroethane	7.65	144	43130	97.27	ppb	94
59) 2-Chloroethyl vinyl ether	7.70	43	72	95.73	ppb #	32
60) Cis-1,3-Dichloropropene	7.82	75	284536	101.09	ppb	95
61) Toluene	8.14	91	763942	94.72	ppb	95
62) Trans-1,3-Dichloropropene	8.40	75	284366	102.32	ppb	97
63) 1,1,2-TCA	8.57	83	111262	89.16	ppb	94
64) 2-Hexanone	8.86	43	75249	97.17	ppb	97
67) 1,2-EDB	9.06	107	176554	91.30	ppb	91
68) Tetrachloroethene	8.69	164	159680	94.30	ppb	98
69) 1-Chlorohexane	9.56	91	145664	100.06	ppb	96
70) 1,1,1,2-Tetrachloroethane	9.65	131	280557	103.18	ppb	98
71) m&p-Xylene	9.79	106	819687	199.23	ppb	98
72) o-Xylene	10.19	106	418040	96.58	ppb	100
73) Styrene	10.20	104	683285	105.81	ppb	97
75) 1,3-Dichloropropane	8.74	76	251787	88.79	ppb	93
76) Dibromochloromethane	8.96	129	278673	98.64	ppb	89

(#) = qualifier out of range (m) = manual integration

1111M30.D M1111W.M Fri Nov 12 09:46:31 2021

Page 2

Data File : M:\MAX\DATA\211111\1111M30.D  
 Acq On : 11 Nov 21 22:25  
 Sample : 100ug/L VOC STD 11/11/21  
 Misc : IS&S 8/4/21

Vial: 10  
 Operator: LP, DG, CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 12 9:06 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:05:35 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
77) Chlorobenzene	9.55	112	600846	95.20	ppb	95
78) Ethylbenzene	9.68	91	968735	96.74	ppb	99
79) Bromoform	10.37	173	232610	99.05	ppb	99
81) Isopropylbenzene	10.56	105	1102475	91.83	ppb	100
82) 1,1,2,2-Tetrachloroethane	10.87	83	175057	85.76	ppb	# 97
83) 1,2,3-Trichloropropane	10.90	110	90959	88.02	ppb	90
84) t-1,4-Dichloro-2-Butene	10.92	53	45329	84.76	ppb	95
85) Bromobenzene	10.84	156	367600	93.09	ppb	90
86) n-Propylbenzene	10.97	91	1127844	95.87	ppb	96
87) 4-Ethyltoluene	11.08	105	1071396	98.36	ppb	97
88) 2-Chlorotoluene	11.04	91	857599	92.17	ppb	96
89) 1,3,5-Trimethylbenzene	11.14	105	968403	95.57	ppb	99
90) 4-Chlorotoluene	11.15	91	856438	92.46	ppb	95
91) Tert-Butylbenzene	11.46	119	604480	107.44	ppb	98
92) 1,2,4-Trimethylbenzene	11.51	105	999392	103.63	ppb	100
93) Sec-Butylbenzene	11.68	105	1149648	106.74	ppb	94
94) p-Isopropyltoluene	11.83	119	1129734	108.74	ppb	97
95) Benzyl Chloride	12.01	91	270909	109.56	ppb	96
96) 1,3-DCB	11.78	146	663876	97.33	ppb	98
97) 1,4-DCB	11.87	146	652535	93.94	ppb	96
98) n-Butylbenzene	12.24	91	767919	95.87	ppb	99
99) 1,2-DCB	12.24	146	668466	100.22	ppb	97
100) Hexachloroethane	12.48	117	192072	108.88	ppb	85
101) 1,2-Dibromo-3-chloropropan	13.01	75	56554	87.97	ppb	93
102) 1,2,4-Trichlorobenzene	13.83	180	328832	96.65	ppb	94
103) Hexachlorobutadiene	14.01	225	316329	100.40	ppb	92
104) Naphthalene	14.08	128	673906	90.41	ppb	99
105) 1,2,3-Trichlorobenzene	14.32	180	427843	92.48	ppb	99

(#) = qualifier out of range (m) = manual integration





VOLATILE ORGANIC ANALYSIS BY  
EPA METHOD 8260B

Form 7

Second Source Calibration

Lab Name: APPL, Inc.

SDG No: \_\_\_\_\_

Case No: \_\_\_\_\_

Date Analyzed: 11/11/2021

Matrix: Water

Instrument: Max

Initial Cal. Date: 11/11/2021

Data File: 1111M32.D

		Compound	MEAN	CCRF	%D	%Drift
1	TM	Chlorotrifluoroethene	0.0000	0.0091	0.00	TM
2	TM	Dichlorodifluoromethane	0.1340	0.1224	8.7	TM
3	TM	Freon 114	0.0911	0.0902	0.97	TM
4	TM**L	Chloromethane	0.0872	0.0759	13	TM**L 3.1
5	TM*	Vinyl chloride	0.0927	0.0908	2.0	TM*
6	TM	2-Chloro-1,1,1-trifluoroethane	0.0000	0.0021	0.00	TM
7	TM	Bromomethane	0.1031	0.0950	7.9	TM
8	TML	Chloroethane	0.0887	0.0529	40	TML 18
9	TM	Dichlorofluoromethane	0.2076	0.2076	0.00	TM
10	TM	Trichlorofluoromethane	0.2656	0.2497	6.0	TM
11	TM	2,2-Dichloro-1,1,1-trifluoroethane	0.0000	0.0227	0.00	TM
12	TM	Acrolein	0.0117	0.0101	14	TM
13	TM	Acetone	0.0301	0.0283	6.0	TM
14	TM	Freon-113	0.1170	0.1106	5.5	TM
15	TM	Acetonitrile	0.0075	0.0070	6.6	TM
16	TML	2-propanol	0.0000	0.0004	0.00	TML
17	TM	1,2-Dichlorotrifluoroethane	0.2076	0.2076	0.00	TM
18	TM*L	1,1-DCE	0.1505	0.1487	1.2	TM*L 6.1
19	TM	t-Butanol	0.0104	0.0102	2.5	TM
20	TM	Methyl Acetate	0.0506	0.0442	13	TM
21	TML	Iodomethane	0.1104	0.1143	3.6	TML 12
22	TML	Acrylonitrile	0.0235	0.0237	0.74	TML 15
23	TML	2-Methylpentane	0.0000	0.0007	0.00	TML
24	TML	Methylene chloride	0.0919	0.1067	16	TML 6.0
25	TM	Carbon disulfide	0.1241	0.1339	7.9	TM
26	TML	Methyl t-butyl ether (MtBE)	0.3315	0.3319	0.10	TML 5.0
27	TM	Trans-1,2-DCE	0.1046	0.1074	2.7	TM
28	TML	3-Methylpentane	0.0636	0.0525	17	TML 9.9
29	TM	Hexane	0.0000	0.0009	0.00	TM
30	TM	Diisopropyl Ether	0.2118	0.2235	5.5	TM
31	TM**	1,1-DCA	0.1740	0.1677	3.6	TM**
32	TM	Ethyl tert Butyl Ether	0.2819	0.2742	2.7	TM
33	TML	Methylcyclopentane	0.0124	0.0089	28	TML 39 *NT
34	TM	MEK (2-Butanone)	0.0324	0.0309	4.8	TM
35	TML	Cis-1,2-DCE	0.1200	0.1179	1.8	TML 6.2
36	TM	2,2-Dichloropropane	0.2277	0.2077	8.8	TM
37	TM*	Chloroform	0.2428	0.2412	0.68	TM*
38	TML	Bromochloromethane	0.1009	0.0969	4.0	TML 4.8
39	TML	1,1,1-TCA	0.2680	0.2655	0.92	TML 4.6
40	TML	Cyclohexane	0.0680	0.0769	13	TML 4.6

Average

6.2

VOLATILE ORGANIC ANALYSIS BY  
EPA METHOD 8260B

Form 7

Second Source Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Date Analyzed: 11/11/2021  
Instrument: Max  
Cal. Date: 11/11/2021  
Data File: 1111M32.D

		Compound	MEAN	CCRF	%D	%Drift
41	TM	1,1-Dichloropropene	0.1416	0.1426	0.71	TM
42	TM	2,2,4-Trimethylpentane	0.1982	0.1810	8.6	TM
43	TM	Carbon Tetrachloride	0.2554	0.2555	0.04	TM
44	TM	Tert Amyl Methyl Ether	0.2880	0.2625	8.9	TM
45	TM	1,2-DCA	0.2342	0.2206	5.8	TM
46	TM	Benzene	0.4057	0.4104	1.2	TM
47	TM	TCE	0.1300	0.1238	4.8	TM
48	TM	2-Pentanone	0.0533	0.0523	1.9	TM
49	TM*	1,2-Dichloropropane	0.0484	0.0431	11	TM*
50	TM	Bromodichloromethane	0.1904	0.1943	2.0	TM
51	TM	Methyl Cyclohexane	0.1466	0.1445	1.4	TM
52	TM	Dibromomethane	0.0784	0.0719	8.3	TM
53	TM	MIBK (methyl isobutyl ketone)	0.0662	0.0660	0.24	TM
54	TML	1-Bromo-2-chloroethane	0.0252	0.0267	6.1	TML 3.1
55	TML	2-Chloroethyl vinyl ether	0.0000	0.0000	0.00	TML
56	TM	Cis-1,3-Dichloropropene	0.1768	0.1766	0.15	TM
57	TM*	Toluene	0.5012	0.4626	7.7	TM*
58	TM	Trans-1,3-Dichloropropene	0.1693	0.1696	0.18	TM
59	TM	1,1,2-TCA	0.0736	0.0636	14	TM
60	TM	2-Hexanone	0.0431	0.0421	2.4	TM
61	TM	1,2-EDB	0.1196	0.1285	7.4	TM
62	TML	Tetrachloroethene	0.1324	0.1129	15	TML 1.5
63	TM	1-Chlorohexane	0.0977	0.0837	14	TM
64	TM	1,1,1,2-Tetrachloroethane	0.2003	0.1920	4.1	TM
65	TM	m&p-Xylene	0.2709	0.2696	0.46	TM
66	TM	o-Xylene	0.2622	0.2720	3.7	TM
67	TM	Styrene	0.4145	0.4416	6.5	TM
68	TML	1,3-Dichloropropane	0.1649	0.1623	1.6	TML 8.6
69	TM	Dibromochloromethane	0.1925	0.1812	5.9	TM
70	TM**	Chlorobenzene	0.4034	0.4083	1.2	TM**
71	TM*	Ethylbenzene	0.6265	0.6531	4.3	TM*
72	TM**	Bromoform	0.1503	0.1462	2.7	TM**
73	TM	Isopropylbenzene	1.066	1.106	3.8	TM
74	TM**	1,1,2,2-Tetrachloroethane	0.1775	0.1527	14	TM**
75	TML	1,2,3-Trichloropropane	0.1011	0.0913	9.6	TML 0.10
76	TML	t-1,4-Dichloro-2-Butene	0.0414	0.0450	8.5	TML 5.9
77	TM	Bromobenzene	0.3809	0.3697	3.0	TM
78	TM	n-Propylbenzene	1.042	1.084	4.0	TM
79	TM	4-Ethyltoluene	1.021	1.040	1.9	TM
80	TM	2-Chlorotoluene	0.8206	0.8619	5.0	TM
		Average			5.1	

VOLATILE ORGANIC ANALYSIS BY  
EPA METHOD 8260B

Form 7

Second Source Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Date Analyzed: 11/11/2021  
Instrument: Max  
Cal. Date: 11/11/2021  
Data File: 1111M32.D

		Compound	MEAN	CCRF	%D	%Drift
81	TM	1,3,5-Trimethylbenzene	0.9005	0.9748	8.2	TM
82	TM	4-Chlorotoluene	0.8292	0.8600	3.7	TM
83	TM	Tert-Butylbenzene	0.5251	0.5461	4.0	TM
84	TM	1,2,4-Trimethylbenzene	0.8840	0.9721	10.0	TM
85	TM	Sec-Butylbenzene	0.9755	1.047	7.3	TM
86	TML	p-Isopropyltoluene	0.9027	0.9877	9.4	TML 3.9
87	TML	Benzyl Chloride	0.2431	0.1833	25	TML 17
88	TM	1,3-DCB	0.6621	0.6753	3.6	TM
89	TM	1,4-DCB	0.6758	0.6211	8.1	TM
90	TML	n-Butylbenzene	0.5559	0.5713	2.8	TML 10
91	TM	1,2-DCB	0.6054	0.6104	0.83	TM
92	TML	Hexachloroethane	0.1637	0.1716	4.9	TML 2.1
93	TML	1,2-Dibromo-3-chloropropane	0.0435	0.0410	5.7	TML 15
94	TML	1,2,4-Trichlorobenzene	0.1844	0.1850	0.36	TML 19
95	TML	Hexachlorobutadiene	0.2201	0.2343	6.5	TML 12
96	TML	Naphthalene	0.3406	0.3295	3.3	TML 16
97	TML	1,2,3-Trichlorobenzene	0.2270	0.2316	2.1	TML 19
98						
99						
100						
101						
102						
103						
104						
105						
106						
107						
108						
109						
110						
111						
112						
113						
114						
115						
116						
117						
118						
119						
120						

Average

6.2

Data File : M:\MAX\DATA\211111\1111M32.D  
 Acq On : 11 Nov 21 23:22  
 Sample : (SS) 10ug/L VOC STD 11/11/21  
 Misc : IS&S 8/4/21

Vial: 12  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 12 9:40 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:40:33 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.37	96	431765	25.00	ppb	0.00
65) Chlorobenzene-D5 (IS)	9.52	117	384615	25.00	ppb	0.00
80) 1,4-Dichlorobenzene-D (IS)	11.84	152	244603	25.00	ppb	0.00
<b>System Monitoring Compounds</b>						
41) Dibromofluoromethane(S)	5.59	111	134844	25.06	ppb	0.00
Spiked Amount	25.000		Recovery	=	100.224%	
46) 1,2-DCA-D4(S)	5.98	65	93416	24.84	ppb	0.00
Spiked Amount	25.000		Recovery	=	99.360%	
66) Toluene-D8(S)	8.08	98	448626	24.55	ppb	0.00
Spiked Amount	25.000		Recovery	=	98.192%	
74) 4-Bromofluorobenzene(S)	10.70	95	178779	25.65	ppb	0.00
Spiked Amount	25.000		Recovery	=	102.608%	
<b>Target Compounds</b>						
3) Dichlorodifluoromethane	1.19	85	21136	9.13	ppb	96
4) Freon 114	1.30	85	15580	9.90	ppb	93
5) Chloromethane	1.34	50	13106	9.69	ppb	100
5) Vinyl chloride	1.43	62	15688	9.80	ppb	# 79
8) Bromomethane	1.69	94	16405	9.21	ppb	95
9) Chloroethane	1.79	64	9130	8.45	ppb	93
10) Dichlorofluoromethane	1.99	67	35849	10.00	ppb	100
11) Trichlorofluoromethane	2.02	101	43130	9.40	ppb	91
13) Acrolein	2.46	56	21752	107.99	ppb	93
14) Acetone	2.63	43	24427	47.00	ppb	90
15) Freon-113	2.55	151	19102	9.45	ppb	93
16) Acetonitrile	2.95	41	15170	116.76	ppb	89
18) 1,2-Dichlorotrifluoroethan	1.99	67	35849	10.00	ppb	100
19) 1,1-DCE	2.53	61	25684	9.39	ppb	91
20) t-Butanol	3.36	59	21955	121.85	ppb	96
21) Methyl Acetate	3.02	43	7631	8.73	ppb	95
22) Iodomethane	2.68	142	19748	8.75	ppb	96
23) Acrylonitrile	3.46	53	4092	8.51	ppb	# 83
25) Methylene chloride	3.12	84	18427	10.60	ppb	98
26) Carbon disulfide	2.74	76	23120	10.79	ppb	98
27) Methyl t-butyl ether (MtBE)	3.50	73	57317	9.50	ppb	94
28) Trans-1,2-DCE	3.46	96	18553	10.27	ppb	87
29) 3-Methylpentane	3.49	57	9070	9.01	ppb	# 93
31) Diisopropyl Ether	4.28	45	38601	10.55	ppb	93
32) 1,1-DCA	4.10	63	28967	9.64	ppb	96
34) Ethyl tert Butyl Ether	4.80	59	47351	9.73	ppb	98
35) Methylcyclopentane	4.80	56	1544	6.06	ppb	100

(#) = qualifier out of range (m) = manual integration

Data File : M:\MAX\DATA\211111\1111M32.D  
 Acq On : 11 Nov 21 23:22  
 Sample : (SS) 10ug/L VOC STD 11/11/21  
 Misc : IS&S 8/4/21

Vial: 12  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 12 9:40 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:40:33 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
36) MEK (2-Butanone)	5.02	43	26648	47.59	ppb	97
37) Cis-1,2-DCE	4.95	96	20360	9.38	ppb	85
38) 2,2-Dichloropropane	4.93	77	35873	9.12	ppb #	91
39) Chloroform	5.39	83	41649	9.93	ppb	84
40) Bromochloromethane	5.26	130	16729	9.52	ppb	95
42) 1,1,1-TCA	5.57	97	45855	9.54	ppb	97
43) Cyclohexane	5.62	41	13289	10.46	ppb	75
44) 1,1-Dichloropropene	5.78	75	24628	10.07	ppb	91
45) 2,2,4-Trimethylpentane	6.15	57	31267	9.14	ppb	94
47) Carbon Tetrachloride	5.77	117	44121	10.00	ppb	93
48) Tert Amyl Methyl Ether	6.21	73	45330	9.11	ppb #	91
49) 1,2-DCA	6.07	62	38093	9.42	ppb	98
50) Benzene	6.03	78	70881	10.12	ppb	91
51) TCE	6.78	95	21374	9.52	ppb	96
52) 2-Pentanone	7.03	43	112882	122.63	ppb	95
53) 1,2-Dichloropropane	7.03	63	7437	8.89	ppb #	93
54) Bromodichloromethane	7.34	83	33556	10.20	ppb	94
55) Methyl Cyclohexane	6.97	83	24953	9.86	ppb	90
56) Dibromomethane	7.15	93	12422	9.17	ppb	91
57) MIBK (methyl isobutyl ket	8.00	43	57036	49.88	ppb	96
58) 1-Bromo-2-chloroethane	7.65	144	4609	9.69	ppb	84
60) Cis-1,3-Dichloropropene	7.82	75	30493	9.99	ppb	92
61) Toluene	8.14	91	79886	9.23	ppb	90
62) Trans-1,3-Dichloropropene	8.40	75	29292	10.02	ppb	89
63) 1,1,2-TCA	8.58	83	10984	8.64	ppb	94
64) 2-Hexanone	8.85	43	36325	48.78	ppb	94
67) 1,2-EDB	9.06	107	19771	10.74	ppb	99
68) Tetrachloroethene	8.69	164	17368	9.85	ppb	94
69) 1-Chlorohexane	9.55	91	12878	8.57	ppb	89
70) 1,1,1,2-Tetrachloroethane	9.64	131	29546	9.59	ppb	91
71) m&p-Xylene	9.79	106	82963	19.91	ppb	93
72) o-Xylene	10.19	106	41841	10.37	ppb	90
73) Styrene	10.20	104	67935	10.65	ppb	98
75) 1,3-Dichloropropane	8.74	76	24967	9.14	ppb	92
76) Dibromochloromethane	8.96	129	27871	9.41	ppb	84
77) Chlorobenzene	9.55	112	62809	10.12	ppb	94
78) Ethylbenzene	9.68	91	100481	10.43	ppb	97
79) Bromoform	10.37	173	22499	9.73	ppb	88
81) Isopropylbenzene	10.56	105	108248	10.38	ppb	100
82) 1,1,2,2-Tetrachloroethane	10.87	83	14938	8.60	ppb #	96
83) 1,2,3-Trichloropropane	10.90	110	8936	10.01	ppb #	60
84) t-1,4-Dichloro-2-Butene	10.92	53	4399	10.59	ppb #	61

(#) = qualifier out of range (m) = manual integration

Data File : M:\MAX\DATA\211111\1111M32.D  
 Acq On : 11 Nov 21 23:22  
 Sample : (SS) 10ug/L VOC STD 11/11/21  
 Misc : IS&S 8/4/21

Vial: 12  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 12 9:40 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:40:33 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
85) Bromobenzene	10.84	156	36168	9.70	ppb	88
86) n-Propylbenzene	10.97	91	106013	10.40	ppb	99
87) 4-Ethyltoluene	11.08	105	101743	10.19	ppb	96
88) 2-Chlorotoluene	11.04	91	84332	10.50	ppb	94
89) 1,3,5-Trimethylbenzene	11.14	105	95376	10.82	ppb	98
90) 4-Chlorotoluene	11.15	91	84147	10.37	ppb	97
91) Tert-Butylbenzene	11.46	119	53432	10.40	ppb	96
92) 1,2,4-Trimethylbenzene	11.51	105	95114	11.00	ppb	95
93) Sec-Butylbenzene	11.68	105	102426	10.73	ppb	94
94) p-Isopropyltoluene	11.83	119	96638	9.61	ppb	95
95) Benzyl Chloride	12.01	91	17937	8.29	ppb	98
96) 1,3-DCB	11.78	146	66072	10.36	ppb	98
97) 1,4-DCB	11.87	146	60765	9.19	ppb	98
98) n-Butylbenzene	12.24	91	55897	8.96	ppb	96
99) 1,2-DCB	12.24	146	59723	10.08	ppb	94
100) Hexachloroethane	12.48	117	16794	9.79	ppb	87
101) 1,2-Dibromo-3-chloropropan	13.02	75	4014	8.53	ppb	87
102) 1,2,4-Trichlorobenzene	13.83	180	18104	8.13	ppb	91
103) Hexachlorobutadiene	14.01	225	22925	8.77	ppb	97
104) Naphthalene	14.08	128	32234	8.40	ppb	94
105) 1,2,3-Trichlorobenzene	14.32	180	22662	8.14	ppb	97

(#) = qualifier out of range (m) = manual integration

QUANTIFICATION REPORT


Data File : M:\MAX\DATA\211111\1111M32.D  
Acq On : 11 Nov 21 23:22  
Sample : (SS) 10ug/L VOC STD 11/11/21  
Misc : IS&S 8/4/21

Vial: 12  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Nov 12 9:40 2021

Quant Results File: M1111W.RES

Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Fri Nov 12 09:40:33 2021  
Response via : Initial Calibration





VOLATILE ORGANIC ANALYSIS  
VOLATILE ORGANIC COMPOUNDS

Form 7

Continuing Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Date Analyzed: 11/19/2021  
Instrument: Thor  
Initial Cal. Date: 11/9/2021  
Data File: 1119T31.D

	Compound	MEAN	CCRF	%D	%Drift
1	I Fluorobenzene (IS)	ISTD			I
2	TML Dichlorodifluoromethane	0.0890	0.0887	0.29	TML 15
3	TMQ Freon 114	0.0545	0.0724	33	TMQ 8.6
4	TM**L Chloromethane	0.0330	0.0223	32	TM**L 18
5	TM*L Vinyl chloride	0.0684	0.0579	15	TM*L 16
6	TML Bromomethane	0.0607	0.0532	12	TML 2.7
7	TML Chloroethane	0.0340	0.0380	12	TML 3.5
8	TML Dichlorofluoromethane	0.1408	0.1660	18	TML 16
9	TM Trichlorofluoromethane	0.2378	0.2490	4.7	TM
10	TM Acrolein	0.0124	0.0049	61	TM *NT
11	TM Acetone	0.0235	0.0223	5.1	TM
12	TM Freon-113	0.0568	0.0529	6.8	TM
13	TM*L 1,1-DCE	0.1398	0.1177	16	TM*L 18
14	TMQ Acetonitrile	0.0012	0.0012	1.2	TMQ 5.5
15	TM t-Butanol	0.0032	0.0028	12	TM
16	TML Methyl Acetate	0.0417	0.0414	0.58	TML 8.3
17	TML Iodomethane	0.0622	0.0524	16	TML 4.8
18	TML Acrylonitrile	0.0146	0.0155	6.3	TML 3.6
19	TML Methylene chloride	0.0836	0.0846	1.2	TML 8.2
20	TML Carbon disulfide	0.1230	0.0926	25	TML 19
21	TM Methyl t-butyl ether (MtBE)	0.2625	0.2841	8.3	TM
22	TML Trans-1,2-DCE	0.1081	0.1006	7.0	TML 17
23	TML Diisopropyl Ether	0.1643	0.1616	1.7	TML 14
24	TM**L 1,1-DCA	0.1390	0.1458	4.9	TM**L 4.5
25	TML Vinyl Acetate	0.1294	0.1287	0.59	TML 19
26	TM Ethyl tert Butyl Ether	0.2262	0.2413	6.7	TM
27	TM MEK (2-Butanone)	0.0302	0.0287	4.8	TM
28	TM Cis-1,2-DCE	0.1314	0.1417	7.9	TM
29	TM 2,2-Dichloropropane	0.1719	0.1954	14	TM
30	TM 2-Methylpentane	0.0000	0.0176	0.00	TM
31	TML 3-Methylpentane	0.0432	0.0464	7.3	TML 4.8
32	TM* Chloroform	0.2008	0.2209	10	TM*
33	TML Bromochloromethane	0.0543	0.0540	0.65	TML 8.7
34	S Dibromofluoromethane(S)	0.2797	0.3210	15	S
35	TM 1,1,1-TCA	0.1032	0.1078	4.5	TM
36	TML Cyclohexane	0.1195	0.1040	13	TML 22 *NT
37	TML 1,1-Dichloropropene	0.1338	0.1288	3.7	TML 11
38	TM 2,2,4-Trimethylpentane	0.2757	0.2247	18	TM
39	S 1,2-DCA-D4(S)	0.2994	0.3368	12	S
40	TML Carbon Tetrachloride	0.2081	0.2658	28	TML 10

Average

11.4

VOLATILE ORGANIC ANALYSIS  
VOLATILE ORGANIC COMPOUNDS

Form 7

Continuing Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Date Analyzed: 11/19/2021  
Instrument: Thor  
Cal. Date: 11/9/2021  
Data File: 1119T31.D

		Compound	MEAN	CCRF	%D	%Drift	
41	TM	Tert Amyl Methyl Ether	0.2710	0.2738	1.0	TM	
42	TML	Methylcyclopentane	0.0097	0.0075	23	TML	31 *NT
43	TM	1,2-DCA	0.1699	0.1704	0.29	TM	
44	TM	Benzene	0.3968	0.3564	10	TM	
45	TM	TCE	0.0925	0.0928	0.27	TM	
46	TM	2-Pentanone	0.0618	0.0543	12	TM	
47	TM*	1,2-Dichloropropane	0.0895	0.0831	7.2	TM*	
48	TM	Bromodichloromethane	0.1636	0.1741	6.4	TM	
49	TM	Methyl Cyclohexane	0.1835	0.1521	17	TM	
50	TML	Dibromomethane	0.1451	0.1750	21	TML	10
51	TM	MIBK (methyl isobutyl ketone)	0.0804	0.0734	8.7	TM	
52	TM	1-Bromo-2-chloroethane	0.0627	0.0523	17	TM	
53	TM	Cis-1,3-Dichloropropene	0.1668	0.1508	9.6	TM	
54	TM*	Toluene	0.5221	0.4966	4.9	TM*	
55	TM	Trans-1,3-Dichloropropene	0.1616	0.1577	2.5	TM	
56	TML	1,1,2-TCA	0.1058	0.1142	7.9	TML	0.89
57	TM	2-Hexanone	0.0563	0.0488	13	TM	
58	I	Chlorobenzene-D5 (IS)	ISTD			I	
59	S	Toluene-D8(S)	0.9832	1.029	4.6	S	
60	TM	1,2-EDB	0.1292	0.1277	1.1	TM	
61	TM	Tetrachloroethene	0.2793	0.2959	5.9	TM	
62	TML	1-Chlorohexane	0.1924	0.1656	14	TML	10
63	TM	1,1,1,2-Tetrachloroethane	0.1799	0.1917	6.6	TM	
64	TM	m&p-Xylene	0.5028	0.4761	5.3	TM	
65	TM	o-Xylene	0.5296	0.5027	5.1	TM	
66	TM	Styrene	0.3906	0.3764	3.6	TM	
67	S	4-Bromofluorobenzene(S)	0.3924	0.4220	7.6	S	
68	TM	1,3-Dichloropropane	0.1660	0.1540	7.2	TM	
69	TM	Dibromochloromethane	0.1778	0.1912	7.5	TM	
70	TM**	Chlorobenzene	0.4416	0.4220	4.4	TM**	
71	TM*	Ethylbenzene	0.6541	0.5981	8.5	TM*	
72	TM**	Bromoform	0.1722	0.1856	7.8	TM**	
73	I	1,4-Dichlorobenzene-D (IS)	ISTD			I	
74	TM	Isopropylbenzene	0.9854	0.9029	8.4	TM	
75	TM**	1,1,2,2-Tetrachloroethane	0.1957	0.1700	13	TM**	
76	TML	1,2,3-Trichloropropane	0.0863	0.0804	6.8	TML	10
77	TML	t-1,4-Dichloro-2-Butene	0.0434	0.0323	25	TML	26 *NT
78	TM	Bromobenzene	0.3619	0.3578	1.1	TM	
79	TM	n-Propylbenzene	1.085	0.9388	13	TM	
80	TM	4-Ethyltoluene	1.007	0.9166	8.9	TM	
Average					8.6		

VOLATILE ORGANIC ANALYSIS  
VOLATILE ORGANIC COMPOUNDS

Form 7

Continuing Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Date Analyzed: 11/19/2021  
Instrument: Thor  
Cal. Date: 11/9/2021  
Data File: 1119T31.D

		Compound	MEAN	CCRF	%D	%Drift
81	TM	2-Chlorotoluene	0.7393	0.6662	9.9	TM
82	TM	1,3,5-Trimethylbenzene	0.8976	0.8039	10	TM
83	TM	4-Chlorotoluene	0.7492	0.7034	6.1	TM
84	TM	Tert-Butylbenzene	0.9345	0.8851	5.3	TM
85	TM	1,2,4-Trimethylbenzene	0.8548	0.7826	8.4	TM
86	TM	Sec-Butylbenzene	1.079	0.9747	9.7	TM
87	TM	p-Isopropyltoluene	1.023	0.9628	5.9	TM
88	TM	Benzyl Chloride	0.3838	0.3358	13	TM
89	TM	1,3-DCB	0.6603	0.6252	5.3	TM
90	TM	1,4-DCB	0.6822	0.6441	5.6	TM
91	TM	n-Butylbenzene	0.7192	0.6539	9.1	TM
92	TM	1,2-DCB	0.6039	0.5789	4.1	TM
93	TML	Hexachloroethane	0.2240	0.2760	23	TML 2.1
94	TML	1,2-Dibromo-3-chloropropane	0.0586	0.0673	15	TML 11
95	TML	1,2,4-Trichlorobenzene	0.4679	0.4693	0.30	TML 4.0
96	TM	Hexachlorobutadiene	0.3204	0.3448	7.6	TM
97	TML	Naphthalene	0.3777	0.3247	14	TML 18
98	TM	1,2,3-Trichlorobenzene	0.4252	0.4167	2.0	TM
99						
100						
101						
102						
103						
104						
105						
106						
107						
108						
109						
110						
111						
112						
113						
114						
115						
116						
117						
118						
119						
120						

Average

8.6

Data File : M:\THOR\DATA\211111\1119T31.D  
 Acq On : 19 Nov 21 22:11  
 Sample : 211119B CCV/LCS 10ug/L  
 Misc : IS&S 8/15/21

Vial: 31  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 22 11:04 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 10:21:13 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.35	96	251289	25.00	ppb	0.00
68) Chlorobenzene-D5 (IS)	9.81	117	252734	25.00	ppb	0.00
83) 1,4-Dichlorobenzene-D (IS)	12.37	152	190553	25.00	ppb	0.00

#### System Monitoring Compounds

43) Dibromofluoromethane(S)	5.49	111	80671	28.69	ppb	0.00
Spiked Amount				25.000		
				Recovery	=	114.760%
48) 1,2-DCA-D4(S)	5.91	65	84645	28.12	ppb	0.00
Spiked Amount				25.000		
				Recovery	=	112.492%
69) Toluene-D8(S)	8.22	98	259983	26.16	ppb	0.00
Spiked Amount				25.000		
				Recovery	=	104.632%
77) 4-Bromofluorobenzene(S)	11.11	95	106666	26.89	ppb	0.00
Spiked Amount				25.000		
				Recovery	=	107.560%

#### Target Compounds

	R.T.	QIon	Response	Conc	Units	Qvalue
3) Dichlorodifluoromethane	1.10	85	8918	11.49	ppb #	87
4) Freon 114	1.20	85	7280	10.86	ppb	96
5) Chloromethane	1.26	50	2239	8.17	ppb	97
6) Vinyl chloride	1.32	62	5815	8.38	ppb #	86
9) Bromomethane	1.59	96	5351	9.73	ppb	96
10) Chloroethane	1.68	64	3821	10.35	ppb	92
11) Dichlorofluoromethane	1.87	67	16687	11.62	ppb	93
12) Trichlorofluoromethane	1.91	101	25025	10.47	ppb	98
16) Acrolein	2.31	56	6149	49.37	ppb	100
17) Acetone	2.48	43	11203	47.45	ppb #	75
18) Freon-113	2.43	101	5317	9.32	ppb	93
19) 1,1-DCE	2.41	61	11835	8.22	ppb #	79
21) Acetonitrile	2.79	40	1507	131.92	ppb	85
22) t-Butanol	3.16	59	3493	110.18	ppb #	89
23) Methyl Acetate	2.87	43	4164	9.17	ppb #	82
24) Iodomethane	2.55	142	5269	9.52	ppb	97
25) Acrylonitrile	3.30	52	1563	9.64	ppb #	85
26) Methylene chloride	2.96	49	8506	9.18	ppb #	77
27) Carbon disulfide	2.61	76	9308	8.10	ppb	99
28) Methyl t-butyl ether (MtBE)	3.34	73	28558	10.83	ppb #	91
29) Trans-1,2-DCE	3.32	61	10110	8.27	ppb	90
31) Diisopropyl Ether	4.12	45	16246	8.60	ppb	91
33) 1,1-DCA	3.92	63	14657	9.55	ppb #	94
34) Vinyl Acetate	4.11	43	12935	8.07	ppb	99
35) Ethyl tert Butyl Ether	4.68	59	24256	10.67	ppb	99
36) MEK (2-Butanone)	4.87	43	14440	47.62	ppb	98
37) Cis-1,2-DCE	4.81	61	14247	10.79	ppb	95

(#) = qualifier out of range (m) = manual integration  
 1119T31.D T1109W.M Mon Nov 22 11:04:26:01 2021

Data File : M:\THOR\DATA\211111\1119T31.D  
 Acq On : 19 Nov 21 22:11  
 Sample : 211119B CCV/LCS 10ug/L  
 Misc : IS&S 8/15/21

Vial: 31  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 22 11:04 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 10:21:13 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
38) 2,2-Dichloropropane	4.79	77	19641	11.37	ppb	100
40) 3-Methylpentane	3.33	57	4664	9.52	ppb	91
41) Chloroform	5.28	83	22208	11.01	ppb	98
42) Bromochloromethane	5.14	49	5425	9.13	ppb #	71
44) 1,1,1-TCA	5.49	97	10836	10.45	ppb	96
45) Cyclohexane	5.55	56	10451	7.85	ppb	86
46) 1,1-Dichloropropene	5.72	75	12950	8.92	ppb	95
47) 2,2,4-Trimethylpentane	6.13	57	22587	8.15	ppb	99
49) Carbon Tetrachloride	5.71	117	26721	11.01	ppb	94
50) Tert Amyl Methyl Ether	6.18	73	27522	10.10	ppb	92
51) Methylcyclopentane	4.67	56	753	6.94	ppb	100
52) 1,2-DCA	6.01	62	17127	10.03	ppb	96
53) Benzene	5.97	78	35821	8.98	ppb	99
54) TCE	6.80	130	9323	10.03	ppb	97
55) 2-Pentanone	7.05	43	68227	109.89	ppb	97
56) 1,2-Dichloropropane	7.05	63	8351	9.28	ppb #	92
57) Bromodichloromethane	7.40	83	17501	10.64	ppb	99
58) Methyl Cyclohexane	7.01	83	15288	8.29	ppb	99
59) Dibromomethane	7.19	174	17592	11.00	ppb	89
60) MIBK (methyl isobutyl ket	8.12	43	36892	45.65	ppb	95
61) 1-Bromo-2-chloroethane	7.73	63	5256	8.34	ppb #	80
63) Cis-1,3-Dichloropropene	7.92	75	15153	9.04	ppb #	88
64) Toluene	8.29	91	49919	9.51	ppb	100
65) Trans-1,3-Dichloropropene	8.56	75	15847	9.75	ppb	98
66) 1,1,2-TCA	8.76	97	11476	10.09	ppb #	84
67) 2-Hexanone	9.06	43	24539	43.33	ppb	96
70) 1,2-EDB	9.29	107	12913	9.89	ppb	97
71) Tetrachloroethene	8.90	166	29909	10.59	ppb	92
72) 1-Chlorohexane	9.85	91	16736	8.98	ppb	89
73) 1,1,1,2-Tetrachloroethane	9.94	131	19382	10.66	ppb	89
74) m&p-Xylene	10.11	91	96259	18.94	ppb	96
75) o-Xylene	10.54	91	50820	9.49	ppb	99
76) Styrene	10.56	104	38048	9.64	ppb	92
78) 1,3-Dichloropropane	8.93	76	15566	9.28	ppb	96
79) Dibromochloromethane	9.17	129	19332	10.75	ppb	90
80) Chlorobenzene	9.85	112	42660	9.56	ppb	96
81) Ethylbenzene	9.98	91	60469	9.15	ppb	100
82) Bromoform	10.74	173	18765	10.78	ppb	91
84) Isopropylbenzene	10.95	105	68821	9.16	ppb	96
85) 1,1,2,2-Tetrachloroethane	11.27	83	12954	8.68	ppb	97
86) 1,2,3-Trichloropropane	11.31	110	6127	8.97	ppb	96
87) t-1,4-Dichloro-2-Butene	11.34	53	2465	7.44	ppb	96

(#) = qualifier out of range (m) = manual integration

Data File : M:\THOR\DATA\211111\1119T31.D  
 Acq On : 19 Nov 21 22:11  
 Sample : 211119B CCV/LCS 10ug/L  
 Misc : IS&S 8/15/21

Vial: 31  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 22 11:04 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 10:21:13 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
88) Bromobenzene	11.26	156	27275	9.89	ppb	94
89) n-Propylbenzene	11.40	91	71558	8.65	ppb	99
90) 4-Ethyltoluene	11.53	105	69866	9.11	ppb	97
91) 2-Chlorotoluene	11.48	91	50781	9.01	ppb	98
92) 1,3,5-Trimethylbenzene	11.60	105	61277	8.96	ppb	97
93) 4-Chlorotoluene	11.60	91	53614	9.39	ppb	99
94) Tert-Butylbenzene	11.95	119	67465	9.47	ppb	97
95) 1,2,4-Trimethylbenzene	12.00	105	59650	9.16	ppb	100
96) Sec-Butylbenzene	12.19	105	74295	9.03	ppb	94
97) p-Isopropyltoluene	12.35	119	73389	9.41	ppb	97
98) Benzyl Chloride	12.55	91	25597	8.75	ppb	95
99) 1,3-DCB	12.30	146	47657	9.47	ppb	98
100) 1,4-DCB	12.40	146	49091	9.44	ppb	98
101) n-Butylbenzene	12.80	91	49839	9.09	ppb	94
102) 1,2-DCB	12.80	146	44121	9.59	ppb	97
103) Hexachloroethane	13.08	201	21037	10.21	ppb	93
104) 1,2-Dibromo-3-chloropropan	13.65	157	5129	8.92	ppb	86
105) 1,2,4-Trichlorobenzene	14.57	180	35772	9.60	ppb	90
106) Hexachlorobutadiene	14.76	225	26282	10.76	ppb	# 87
107) Naphthalene	14.83	128	24752	8.18	ppb	96
108) 1,2,3-Trichlorobenzene	15.09	180	31759	9.80	ppb	91



VOLATILE ORGANIC ANALYSIS BY  
EPA METHOD 8260B

Form 7

Continuing Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Date Analyzed: 11/15/2021  
Instrument: Max  
Initial Cal. Date: 11/11/2021  
Data File: 1115M03.D

		Compound	MEAN	CCRF	%D	%Drift
1	I	Fluorobenzene (IS)	ISTD			I
2	TM	Chlorotrifluoroethene	0.0000	0.0110	0.00	TM
3	TM	Dichlorodifluoromethane	0.1340	0.1099	18	TM
4	TM	Freon 114	0.0911	0.0980	7.6	TM
5	TM**L	Chloromethane	0.0872	0.0779	11	TM**L 0.52
6	TM*	Vinyl chloride	0.0927	0.0842	9.1	TM*
7	TM	2-Chloro-1,1,1-trifluoroethane	0.0000	0.0021	0.00	TM
8	TM	Bromomethane	0.1031	0.0940	8.9	TM
9	TML	Chloroethane	0.0887	0.0591	33	TML 4.3
10	TM	Dichlorofluoromethane	0.2076	0.2205	6.2	TM
11	TM	Trichlorofluoromethane	0.2656	0.2603	2.0	TM
12	TM	2,2-Dichloro-1,1,1-trifluoroethane	0.0000	0.0259	0.00	TM
13	TM	Acrolein	0.0117	0.0110	5.8	TM
14	TM	Acetone	0.0301	0.0266	12	TM
15	TM	Freon-113	0.1170	0.1162	0.63	TM
16	TM	Acetonitrile	0.0075	0.0073	3.5	TM
17	TML	2-propanol	0.0000	0.0003	0.00	TML
18	TM	1,2-Dichlorotrifluoroethane	0.2076	0.2205	6.2	TM
19	TM*L	1,1-DCE	0.1505	0.1444	4.0	TM*L 8.8
20	TM	t-Butanol	0.0104	0.0089	15	TM
21	TM	Methyl Acetate	0.0506	0.0481	4.9	TM
22	TML	Iodomethane	0.1104	0.1191	7.9	TML 9.3
23	TML	Acrylonitrile	0.0235	0.0295	25	TML 6.4
24	TML	Methylene chloride	0.0919	0.1042	13	TML 3.6
25	TM	Carbon disulfide	0.1241	0.1195	3.6	TM
26	TML	Methyl t-butyl ether (MtBE)	0.3315	0.3642	9.9	TML 4.8
27	TM	Trans-1,2-DCE	0.1046	0.1060	1.4	TM
28	TML	3-Methylpentane	0.0636	0.0668	4.6	TML 16
29	TM	Hexane	0.0000	0.0001	0.00	TM
30	TM	Diisopropyl Ether	0.2118	0.2288	8.0	TM
31	TM**	1,1-DCA	0.1740	0.1715	1.4	TM**
32	TM	Ethyl tert Butyl Ether	0.2819	0.3216	14	TM
33	TML	Methylcyclopentane	0.0124	0.0146	18	TML 15
34	TM	MEK (2-Butanone)	0.0324	0.0327	1.0	TM
35	TML	Cis-1,2-DCE	0.1200	0.1253	4.4	TML 0.04
36	TM	2,2-Dichloropropane	0.2277	0.2509	10	TM
37	TM*	Chloroform	0.2428	0.2505	3.2	TM*
38	TML	Bromochloromethane	0.1009	0.1048	3.9	TML 3.5
39	S	Dibromofluoromethane(S)	0.3116	0.3086	0.98	S
40	TML	1,1,1-TCA	0.2680	0.2760	3.0	TML 0.60

Average

7.2



VOLATILE ORGANIC ANALYSIS BY  
EPA METHOD 8260B

Form 7

Continuing Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Date Analyzed: 11/15/2021  
Instrument: Max  
Cal. Date: 11/11/2021  
Data File: 1115M03.D

		Compound	MEAN	CCRF	%D		%Drift
41	TML	Cyclohexane	0.0680	0.0703	3.5	TML	4.5
42	TM	1,1-Dichloropropene	0.1416	0.1489	5.1	TM	
43	TM	2,2,4-Trimethylpentane	0.1982	0.1998	0.85	TM	
44	S	1,2-DCA-D4(S)	0.2178	0.2148	1.3	S	
45	TM	Carbon Tetrachloride	0.2554	0.2696	5.6	TM	
46	TM	Tert Amyl Methyl Ether	0.2880	0.3128	8.6	TM	
47	TM	1,2-DCA	0.2342	0.2354	0.52	TM	
48	TM	Benzene	0.4057	0.4211	3.8	TM	
49	TM	TCE	0.1300	0.1318	1.4	TM	
50	TM	2-Pentanone	0.0533	0.0547	2.7	TM	
51	TM*	1,2-Dichloropropane	0.0484	0.0431	11	TM*	
52	TM	Bromodichloromethane	0.1904	0.2021	6.2	TM	
53	TM	Methyl Cyclohexane	0.1466	0.1551	5.8	TM	
54	TM	Dibromomethane	0.0784	0.0810	3.3	TM	
55	TM	MIBK (methyl isobutyl ketone)	0.0662	0.0650	1.9	TM	
56	TML	1-Bromo-2-chloroethane	0.0252	0.0250	0.56	TML	9.3
57	TML	2-Chloroethyl vinyl ether	0.0000	0.0000	0.00	TML	
58	TM	Cis-1,3-Dichloropropene	0.1768	0.1766	0.11	TM	
59	TM*	Toluene	0.5012	0.5178	3.3	TM*	
60	TM	Trans-1,3-Dichloropropene	0.1693	0.1926	14	TM	
61	TM	1,1,2-TCA	0.0736	0.0645	12	TM	
62	TM	2-Hexanone	0.0431	0.0461	7.0	TM	
63	I	Chlorobenzene-D5 (IS)	ISTD			I	
64	S	Toluene-D8(S)	1.188	1.160	2.3	S	
65	TM	1,2-EDB	0.1196	0.1274	6.5	TM	
66	TML	Tetrachloroethene	0.1324	0.1148	13	TML	0.25
67	TM	1-Chlorohexane	0.0977	0.1014	3.9	TM	
68	TM	1,1,1,2-Tetrachloroethane	0.2003	0.1931	3.6	TM	
69	TM	m&p-Xylene	0.2709	0.2779	2.6	TM	
70	TM	o-Xylene	0.2622	0.2776	5.9	TM	
71	TM	Styrene	0.4145	0.4480	8.1	TM	
72	S	4-Bromofluorobenzene(S)	0.4530	0.4423	2.4	S	
73	TML	1,3-Dichloropropane	0.1649	0.1887	14	TML	6.7
74	TM	Dibromochloromethane	0.1925	0.2020	4.9	TM	
75	TM**	Chlorobenzene	0.4034	0.4229	4.8	TM**	
76	TM*	Ethylbenzene	0.6265	0.6692	6.8	TM*	
77	TM**	Bromoform	0.1503	0.1647	9.6	TM**	
78	I	1,4-Dichlorobenzene-D (IS)	ISTD			I	
79	TM	Isopropylbenzene	1.066	1.135	6.5	TM	
80	TM**	1,1,2,2-Tetrachloroethane	0.1775	0.1830	3.1	TM**	

Average

5.2

VOLATILE ORGANIC ANALYSIS BY  
EPA METHOD 8260B

Form 7

Continuing Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Date Analyzed: 11/15/2021  
Instrument: Max  
Cal. Date: 11/11/2021  
Data File: 1115M03.D

		Compound	MEAN	CCRF	%D	%Drift	
81	TML	1,2,3-Trichloropropane	0.1011	0.1014	0.30	TML	12
82	TML	t-1,4-Dichloro-2-Butene	0.0414	0.0468	13	TML	10
83	TM	Bromobenzene	0.3809	0.3686	3.2	TM	
84	TM	n-Propylbenzene	1.042	1.100	5.5	TM	
85	TM	4-Ethyltoluene	1.021	1.052	3.0	TM	
86	TM	2-Chlorotoluene	0.8206	0.8824	7.5	TM	
87	TM	1,3,5-Trimethylbenzene	0.9005	0.9955	11	TM	
88	TM	4-Chlorotoluene	0.8292	0.8887	7.2	TM	
89	TM	Tert-Butylbenzene	0.5251	0.5985	14	TM	
90	TM	1,2,4-Trimethylbenzene	0.8840	0.9581	8.4	TM	
91	TM	Sec-Butylbenzene	0.9755	1.085	11	TM	
92	TML	p-Isopropyltoluene	0.9027	0.9894	9.6	TML	3.8
93	TML	Benzyl Chloride	0.2431	0.2793	15	TML	20
94	TM	1,3-DCB	0.6521	0.6475	0.71	TM	
95	TM	1,4-DCB	0.6758	0.6194	8.3	TM	
96	TML	n-Butylbenzene	0.5559	0.5717	2.8	TML	10
97	TM	1,2-DCB	0.6054	0.6446	6.5	TM	
98	TML	Hexachloroethane	0.1637	0.1929	18	TML	9.3
99	TML	1,2-Dibromo-3-chloropropane	0.0435	0.0481	11	TML	1.8
100	TML	1,2,4-Trichlorobenzene	0.1844	0.1886	2.3	TML	18
101	TML	Hexachlorobutadiene	0.2201	0.2443	11	TML	9.1
102	TML	Naphthalene	0.3406	0.3362	1.3	TML	15
103	TML	1,2,3-Trichlorobenzene	0.2270	0.2300	1.3	TML	19
104							
105							
106							
107							
108							
109							
110							
111							
112							
113							
114							
115							
116							
117							
118							
119							
120							

Average

7.5

Data File : M:\MAX\DATA\211111\1115M03.D  
 Acq On : 15 Nov 21 9:28  
 Sample : 211115A CCV/LCS 10ug/L  
 Misc : IS&S 8/4/21

Vial: 3  
 Operator: LP, DG, CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 15 10:39 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:40:33 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.38	96	414024	25.00	ppb	0.00
65) Chlorobenzene-D5 (IS)	9.53	117	371836	25.00	ppb	0.00
80) 1,4-Dichlorobenzene-D (IS)	11.85	152	236811	25.00	ppb	0.00

System Monitoring Compounds

41) Dibromofluoromethane (S)	5.60	111	127751	24.76	ppb	0.00
Spiked Amount			25.000	Recovery =		99.024%
46) 1,2-DCA-D4 (S)	5.98	65	88952	24.67	ppb	0.00
Spiked Amount			25.000	Recovery =		98.668%
66) Toluene-D8 (S)	8.08	98	431362	24.41	ppb	0.00
Spiked Amount			25.000	Recovery =		97.656%
74) 4-Bromofluorobenzene (S)	10.71	95	164453	24.41	ppb	0.00
Spiked Amount			25.000	Recovery =		97.628%

Target Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
3) Dichlorodifluoromethane	1.20	85	18200	8.20	ppb	100
4) Freon 114	1.30	85	16232	10.76	ppb	98
5) Chloromethane	1.34	50	12901	9.95	ppb	94
6) Vinyl chloride	1.43	62	13948	9.09	ppb #	78
8) Bromomethane	1.70	94	15565	9.11	ppb	94
9) Chloroethane	1.79	64	9784	9.57	ppb	98
10) Dichlorofluoromethane	1.99	67	36521	10.62	ppb	99
11) Trichlorofluoromethane	2.03	101	43103	9.80	ppb	97
13) Acrolein	2.46	56	22739	117.73	ppb #	81
14) Acetone	2.64	43	22016	44.18	ppb	99
15) Freon-113	2.55	151	19252	9.94	ppb #	87
16) Acetonitrile	2.95	41	15024	120.59	ppb #	90
18) 1,2-Dichlorotrifluoroethan	1.99	67	36521	10.62	ppb	100
19) 1,1-DCE	2.54	61	23911	9.12	ppb	93
20) t-Butanol	3.38	59	18409	106.55	ppb #	90
21) Methyl Acetate	3.03	43	7974	9.51	ppb	95
22) Iodomethane	2.69	142	19724	9.07	ppb	90
23) Acrylonitrile	3.48	53	4886	10.64	ppb #	76
25) Methylene chloride	3.12	84	17264	10.36	ppb	92
26) Carbon disulfide	2.74	76	19800	9.64	ppb #	90
27) Methyl t-butyl ether (MtBE)	3.50	73	60319	10.48	ppb	100
28) Trans-1,2-DCE	3.47	96	17555	10.14	ppb	99
29) 3-Methylpentane	3.50	57	11023	11.58	ppb	98
31) Diisopropyl Ether	4.29	45	37888	10.80	ppb	97
32) 1,1-DCA	4.10	63	28402	9.86	ppb	99
34) Ethyl tert Butyl Ether	4.81	59	53252	11.41	ppb	92
35) Methylcyclopentane	4.81	56	2414	11.50	ppb	100

(#) = qualifier out of range (m) = manual integration

Data File : M:\MAX\DATA\211111\1115M03.D  
 Acq On : 15 Nov 21 9:28  
 Sample : 211115A CCV/LCS 10ug/L  
 Misc : IS&S 8/4/21

Vial: 3  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 15 10:39 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:40:33 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
36) MEK (2-Butanone)	5.03	43	27117	50.50	ppb	96
37) Cis-1,2-DCE	4.95	96	20751	10.00	ppb	95
38) 2,2-Dichloropropane	4.94	77	41547	11.02	ppb	99
39) Chloroform	5.40	83	41484	10.32	ppb	90
40) Bromochloromethane	5.26	130	17362	10.35	ppb	96
42) 1,1,1-TCA	5.58	97	45706	9.94	ppb	92
43) Cyclohexane	5.63	41	11648	9.55	ppb	85
44) 1,1-Dichloropropene	5.80	75	24656	10.51	ppb	88
45) 2,2,4-Trimethylpentane	6.15	57	33094	10.08	ppb	# 81
47) Carbon Tetrachloride	5.78	117	44649	10.56	ppb	97
48) Tert Amyl Methyl Ether	6.22	73	51804	10.86	ppb	95
49) 1,2-DCA	6.08	62	38990	10.05	ppb	97
50) Benzene	6.03	78	69735	10.38	ppb	94
51) TCE	6.79	95	21830	10.14	ppb	97
52) 2-Pentanone	7.04	43	113303	128.36	ppb	97
53) 1,2-Dichloropropane	7.03	63	7139	8.90	ppb	95
54) Bromodichloromethane	7.35	83	33476	10.62	ppb	94
55) Methyl Cyclohexane	6.98	83	25689	10.58	ppb	88
56) Dibromomethane	7.16	93	13420	10.33	ppb	92
57) MIBK (methyl isobutyl ket	8.01	43	53795	49.06	ppb	95
58) 1-Bromo-2-chloroethane	7.65	144	4144	9.07	ppb	99
60) Cis-1,3-Dichloropropene	7.82	75	29252	9.99	ppb	97
61) Toluene	8.15	91	85754	10.33	ppb	100
62) Trans-1,3-Dichloropropene	8.40	75	31893	11.38	ppb	93
63) 1,1,2-TCA	8.58	83	10676	8.75	ppb	# 79
64) 2-Hexanone	8.86	43	38195	53.49	ppb	99
67) 1,2-EDB	9.06	107	18944	10.65	ppb	95
68) Tetrachloroethene	8.70	164	17072	10.03	ppb	95
69) 1-Chlorohexane	9.56	91	15085	10.39	ppb	98
70) 1,1,1,2-Tetrachloroethane	9.65	131	28726	9.64	ppb	95
71) m&p-Xylene	9.80	106	82678	20.52	ppb	97
72) o-Xylene	10.19	106	41283	10.59	ppb	96
73) Styrene	10.21	104	66633	10.81	ppb	97
75) 1,3-Dichloropropane	8.74	76	28063	10.67	ppb	94
76) Dibromochloromethane	8.97	129	30040	10.49	ppb	83
77) Chlorobenzene	9.56	112	62895	10.48	ppb	95
78) Ethylbenzene	9.68	91	99528	10.68	ppb	91
79) Bromoform	10.38	173	24498	10.96	ppb	92
81) Isopropylbenzene	10.56	105	107531	10.65	ppb	97
82) 1,1,2,2-Tetrachloroethane	10.87	83	17332	10.31	ppb	# 90
83) 1,2,3-Trichloropropane	10.91	110	9604	11.15	ppb	# 83
84) t-1,4-Dichloro-2-Butene	10.93	53	4431	11.01	ppb	95

(#) = qualifier out of range (m) = manual integration

Data File : M:\MAX\DATA\211111\1115M03.D  
Acq On : 15 Nov 21 9:28  
Sample : 211115A CCV/LCS 10ug/L  
Misc : IS&S 8/4/21

Vial: 3  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Nov 15 10:39 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Fri Nov 12 09:40:33 2021  
Response via : Initial Calibration  
DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
85) Bromobenzene	10.84	156	34911	9.68	ppb	91
86) n-Propylbenzene	10.97	91	104188	10.55	ppb	97
87) 4-Ethyltoluene	11.09	105	99611	10.30	ppb	97
88) 2-Chlorotoluene	11.04	91	83586	10.75	ppb	99
89) 1,3,5-Trimethylbenzene	11.15	105	94299	11.05	ppb	98
90) 4-Chlorotoluene	11.15	91	84184	10.72	ppb	93
91) Tert-Butylbenzene	11.47	119	56696	11.40	ppb	95
92) 1,2,4-Trimethylbenzene	11.52	105	90757	10.84	ppb	100
93) Sec-Butylbenzene	11.69	105	102755	11.12	ppb	98
94) p-Isopropyltoluene	11.84	119	93725	9.62	ppb	96
95) Benzyl Chloride	12.02	91	26459	11.96	ppb	99
96) 1,3-DCB	11.78	146	61334	9.93	ppb	97
97) 1,4-DCB	11.87	146	58677	9.17	ppb	95
98) n-Butylbenzene	12.25	91	54156	8.97	ppb	99
99) 1,2-DCB	12.24	146	61062	10.65	ppb	96
100) Hexachloroethane	12.49	117	18271	10.93	ppb	83
101) 1,2-Dibromo-3-chloropropan	13.02	75	4556	9.82	ppb	93
102) 1,2,4-Trichlorobenzene	13.84	180	17864	8.24	ppb	91
103) Hexachlorobutadiene	14.02	225	23139	9.09	ppb	96
104) Naphthalene	14.08	128	31845	8.50	ppb	96
105) 1,2,3-Trichlorobenzene	14.32	180	21787	8.11	ppb	84

(#) = qualifier out of range (m) = manual integration  
1115M03.D M1111W.M Tue Nov 16 08:00:00 2021

Page 3

Quantitation Report


Data File : M:\MAX\DATA\211111\1115M03.D  
Acq On : 15 Nov 21 9:28  
Sample : 211115A CCV/LCS 10ug/L  
Misc : IS&S 8/4/21

Vial: 3  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Nov 15 10:39 2021

Quant Results File: M1111W.RES

Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Fri Nov 12 09:40:33 2021  
Response via : Initial Calibration



VOLATILE ORGANIC ANALYSIS  
VOLATILE ORGANIC COMPOUNDS

Form 7

Ending Continuing Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Date Analyzed: 11/20/2021  
Instrument: Thor  
Initial Cal. Date: 11/9/2021  
Data File: 1119T52.D

	Compound	MEAN	CCRF	%D	%Drift
1	I Fluorobenzene (IS)	ISTD			I
2	TML Dichlorodifluoromethane	0.0890	0.0627	30	TML 20
3	TMQ Freon 114	0.0545	0.0803	47	TMQ 20
4	TM**L Chloromethane	0.0330	0.0235	29	TM**L 13
5	TM*L Vinyl chloride	0.0684	0.0613	10	TM*L 11
6	L Butane	0.0000	0.0008	0.00	L
7	TML Bromomethane	0.0607	0.0599	1.4	TML 11
8	TML Chloroethane	0.0340	0.0421	24	TML 17
9	TML Dichlorofluoromethane	0.1408	0.1713	22	TML 20
10	TM Trichlorofluoromethane	0.2378	0.2707	14	TM
11	TM Acrolein	0.0124	0.0046	63	TM
12	TM Acetone	0.0235	0.0233	0.92	TM
13	TM Freon-113	0.0568	0.0543	4.3	TM
14	TM*L 1,1-DCE	0.1398	0.1321	5.5	TM*L 8.0
15	TMQ Acetonitrile	0.0012	0.0011	13	TMQ 12
16	TM t-Butanol	0.0032	0.0031	0.82	TM
17	TML Methyl Acetate	0.0417	0.0465	11	TML 0.78
18	TML Iodomethane	0.0622	0.0454	27	TML 18
19	TML Acrylonitrile	0.0146	0.0163	11	TML 0.37
20	TML Methylene chloride	0.0836	0.0945	13	TML 2.5
21	TML Carbon disulfide	0.1230	0.0885	28	TML 23
22	TM Methyl t-butyl ether (MtBE)	0.2625	0.3026	15	TM
23	TML Trans-1,2-DCE	0.1081	0.1137	5.1	TML 7.0
24	TML Diisopropyl Ether	0.1643	0.1805	9.8	TML 4.6
25	TM**L 1,1-DCA	0.1390	0.1495	7.6	TM**L 2.2
26	TML Vinyl Acetate	0.1294	0.1107	14	TML 29
27	TM Ethyl tert Butyl Ether	0.2262	0.2443	8.0	TM
28	TM MEK (2-Butanone)	0.0302	0.0273	9.5	TM
29	TM Cis-1,2-DCE	0.1314	0.1471	12	TM
30	TM 2,2-Dichloropropane	0.1719	0.1911	11	TM
31	TM 2-Methylpentane	0.0000	0.0194	0.00	TM
32	TML 3-Methylpentane	0.0432	0.0477	10	TML 2.4
33	TM* Chloroform	0.2008	0.2330	16	TM*
34	TML Bromochloromethane	0.0543	0.0568	4.6	TML 4.0
35	S Dibromofluoromethane(S)	0.2797	0.3261	17	S
36	TM 1,1,1-TCA	0.1032	0.1166	13	TM
37	TML Cyclohexane	0.1195	0.1033	14	TML 22
38	TML 1,1-Dichloropropene	0.1338	0.1389	3.8	TML 4.3
39	TM 2,2,4-Trimethylpentane	0.2757	0.2206	20	TM
40	S 1,2-DCA-D4(S)	0.2994	0.3414	14	S

\*NT

Average

14.3

VOLATILE ORGANIC ANALYSIS  
VOLATILE ORGANIC COMPOUNDS

Form 7

Ending Continuing Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Date Analyzed: 11/20/2021  
Instrument: Thor  
Cal. Date: 11/9/2021  
Data File: 1119T52.D

		Compound	MEAN	CCRF	%D	%Drift
41	TML	Carbon Tetrachloride	0.2081	0.2932	41	TML 21
42	TM	Tert Amyl Methyl Ether	0.2710	0.2824	4.2	TM
43	TML	Methylcyclopentane	0.0097	0.0102	5.2	TML 6.6
44	TM	1,2-DCA	0.1699	0.1796	5.7	TM
45	TM	Benzene	0.3968	0.3788	4.5	TM
46	TM	TCE	0.0925	0.1016	9.8	TM
47	TM	2-Pentanone	0.0618	0.0543	12	TM
48	TM*	1,2-Dichloropropane	0.0895	0.0945	5.6	TM*
49	TM	Bromodichloromethane	0.1636	0.1883	15	TM
50	TM	Methyl Cyclohexane	0.1835	0.1720	6.3	TM
51	TML	Dibromomethane	0.1451	0.1790	23	TML 12
52	TM	MIBK (methyl isobutyl ketone)	0.0804	0.0710	12	TM
53	TM	1-Bromo-2-chloroethane	0.0627	0.0583	6.9	TM
54	TM	Cis-1,3-Dichloropropene	0.1668	0.1636	1.9	TM
55	TM*	Toluene	0.5221	0.5284	1.2	TM*
56	TM	Trans-1,3-Dichloropropene	0.1616	0.1638	1.4	TM
57	TML	1,1,2-TCA	0.1058	0.1173	11	TML 3.5
58	TM	2-Hexanone	0.0563	0.0499	11	TM
59	I	Chlorobenzene-D5 (IS)	ISTD			I
60	S	Toluene-D8(S)	0.9832	1.014	3.2	S
61	TM	1,2-EDB	0.1292	0.1345	4.2	TM
62	TM	Tetrachloroethene	0.2793	0.2950	5.6	TM
63	TML	1-Chlorohexane	0.1924	0.1650	14	TML 11
64	TM	1,1,1,2-Tetrachloroethane	0.1799	0.2132	19	TM
65	TM	m&p-Xylene	0.5028	0.5052	0.47	TM
66	TM	o-Xylene	0.5296	0.5108	3.5	TM
67	TM	Styrene	0.3906	0.4009	2.6	TM
68	S	4-Bromofluorobenzene(S)	0.3924	0.4115	4.9	S
69	TM	1,3-Dichloropropane	0.1660	0.1674	0.85	TM
70	TM	Dibromochloromethane	0.1778	0.1989	12	TM
71	TM**	Chlorobenzene	0.4416	0.4427	0.26	TM**
72	TM*	Ethylbenzene	0.6541	0.6415	1.9	TM*
73	TM**	Bromoform	0.1722	0.1900	10	TM**
74	I	1,4-Dichlorobenzene-D (IS)	ISTD			I
75	TM	Isopropylbenzene	0.9854	0.9624	2.3	TM
76	TM**	1,1,2,2-Tetrachloroethane	0.1957	0.1577	19	TM**
77	TML	1,2,3-Trichloropropane	0.0863	0.0823	4.5	TML 8.2
78	TML	t-1,4-Dichloro-2-Butene	0.0434	0.0360	17	TML 19
79	TM	Bromobenzene	0.3619	0.3660	1.1	TM
80	TM	n-Propylbenzene	1.085	0.9553	12	TM

Average

8.3



VOLATILE ORGANIC ANALYSIS  
VOLATILE ORGANIC COMPOUNDS

Form 7

Ending Continuing Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Date Analyzed: 11/20/2021  
Instrument: Thor  
Cal. Date: 11/9/2021  
Data File: 1119T52.D

		Compound	MEAN	CCRF	%D		%Drift
81	TM	4-Ethyltoluene	1.007	0.9255	8.1	TM	
82	TM	2-Chlorotoluene	0.7393	0.6904	6.6	TM	
83	TM	1,3,5-Trimethylbenzene	0.8976	0.8171	9.0	TM	
84	TM	4-Chlorotoluene	0.7492	0.7081	5.5	TM	
85	TM	Tert-Butylbenzene	0.9345	0.9439	1.0	TM	
86	TM	1,2,4-Trimethylbenzene	0.8548	0.8115	5.1	TM	
87	TM	Sec-Butylbenzene	1.079	1.011	6.3	TM	
88	TM	p-Isopropyltoluene	1.023	0.9948	2.7	TM	
89	TM	Benzyl Chloride	0.3838	0.2627	32	TM	
90	TM	1,3-DCB	0.6603	0.6420	2.8	TM	
91	TM	1,4-DCB	0.6822	0.6417	5.9	TM	
92	TM	n-Butylbenzene	0.7192	0.6483	9.9	TM	
93	TM	1,2-DCB	0.6039	0.5922	1.9	TM	
94	TML	Hexachloroethane	0.2240	0.2902	30	TML	6.9
95	TML	1,2-Dibromo-3-chloropropane	0.0586	0.0615	5.1	TML	17
96	TML	1,2,4-Trichlorobenzene	0.4679	0.4613	1.4	TML	5.5
97	TM	Hexachlorobutadiene	0.3204	0.3364	5.0	TM	
98	TML	Naphthalene	0.3777	0.3072	19	TML	22
99	TM	1,2,3-Trichlorobenzene	0.4252	0.4206	1.1	TM	
100							
101							
102							
103							
104							
105							
106							
107							
108							
109							
110							
111							
112							
113							
114							
115							
116							
117							
118							
119							
120							

Average

8.3

Data File : M:\THOR\DATA\211111\1119T52.D  
 Acq On : 20 Nov 21 6:47  
 Sample : Ending CCV 10ug/L 11/19/21  
 Misc : IS&S 8/15/21

Vial: 52  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 22 11:04 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 10:21:13 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.34	96	252617	25.00	ppb	0.00
68) Chlorobenzene-D5 (IS)	9.81	117	260147	25.00	ppb	0.00
83) 1,4-Dichlorobenzene-D (IS)	12.37	152	196942	25.00	ppb	0.00

System Monitoring Compounds

43) Dibromofluoromethane (S)	5.49	111	82381	29.14	ppb	0.00
Spiked Amount				25.000		
				Recovery	=	116.576%
48) 1,2-DCA-D4 (S)	5.91	65	86256	28.51	ppb	0.00
Spiked Amount				25.000		
				Recovery	=	114.032%
69) Toluene-D8 (S)	8.22	98	263879	25.79	ppb	0.00
Spiked Amount				25.000		
				Recovery	=	103.172%
77) 4-Bromofluorobenzene (S)	11.11	95	107045	26.22	ppb	0.00
Spiked Amount				25.000		
				Recovery	=	104.868%

Target Compounds

	R.T.	QIon	Response	Conc	Units	Qvalue
3) Dichlorodifluoromethane	1.09	85	6335	8.00	ppb	98
4) Freon 114	1.20	85	8114	12.03	ppb	86
5) Chloromethane	1.27	50	2379	8.67	ppb	100
6) Vinyl chloride	1.33	62	6194	8.88	ppb	99
9) Bromomethane	1.60	96	6050	11.05	ppb	97
10) Chloroethane	1.68	64	4256	11.70	ppb	# 80
11) Dichlorofluoromethane	1.87	67	17306	12.03	ppb	94
12) Trichlorofluoromethane	1.91	101	27357	11.39	ppb	100
16) Acrolein	2.31	56	5868	46.86	ppb	93
17) Acetone	2.48	43	11758	49.54	ppb	# 87
18) Freon-113	2.43	101	5489	9.57	ppb	86
19) 1,1-DCE	2.41	61	13350	9.20	ppb	# 80
21) Acetonitrile	2.79	40	1327	110.51	ppb	84
22) t-Butanol	3.16	59	3951	123.98	ppb	93
23) Methyl Acetate	2.87	43	4694	10.08	ppb	92
24) Iodomethane	2.55	142	4584	8.20	ppb	98
25) Acrylonitrile	3.30	52	1647	9.96	ppb	89
26) Methylene chloride	2.96	49	9552	10.25	ppb	85
27) Carbon disulfide	2.61	76	8946	7.70	ppb	96
28) Methyl t-butyl ether (MtBE)	3.33	73	30581	11.53	ppb	95
29) Trans-1,2-DCE	3.31	61	11486	9.30	ppb	91
31) Diisopropyl Ether	4.11	45	18237	9.54	ppb	95
33) 1,1-DCA	3.91	63	15110	9.78	ppb	96
34) Vinyl Acetate	4.11	43	11185	7.10	ppb	97
35) Ethyl tert Butyl Ether	4.67	59	24686	10.80	ppb	100
36) MEK (2-Butanone)	4.87	43	13789	45.24	ppb	98
37) Cis-1,2-DCE	4.81	61	14859	11.19	ppb	# 87

(#) = qualifier out of range (m) = manual integration

Data File : M:\THOR\DATA\211111\1119T52.D  
 Acq On : 20 Nov 21 6:47  
 Sample : Ending CCV 10ug/L 11/19/21  
 Misc : IS&S 8/15/21

Vial: 52  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 22 11:04 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 10:21:13 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
38) 2,2-Dichloropropane	4.80	77	19311	11.12	ppb	100
40) 3-Methylpentane	3.33	57	4816	9.76	ppb #	93
41) Chloroform	5.29	83	23546	11.61	ppb	97
42) Bromochloromethane	5.14	49	5740	9.60	ppb #	75
44) 1,1,1-TCA	5.49	97	11786	11.30	ppb	90
45) Cyclohexane	5.55	56	10438	7.80	ppb #	82
46) 1,1-Dichloropropene	5.72	75	14032	9.57	ppb	93
47) 2,2,4-Trimethylpentane	6.13	57	22292	8.00	ppb	99
49) Carbon Tetrachloride	5.71	117	29627	12.06	ppb	97
50) Tert Amyl Methyl Ether	6.18	73	28533	10.42	ppb	91
51) Methylcyclopentane	4.67	56	1029	9.34	ppb	100
52) 1,2-DCA	6.01	62	18150	10.57	ppb #	94
53) Benzene	5.97	78	38272	9.55	ppb	98
54) TCE	6.80	130	10267	10.98	ppb	96
55) 2-Pentanone	7.05	43	68599	109.91	ppb	100
56) 1,2-Dichloropropane	7.05	63	9549	10.56	ppb #	96
57) Bromodichloromethane	7.40	83	19031	11.51	ppb	99
58) Methyl Cyclohexane	7.02	83	17380	9.37	ppb #	83
59) Dibromomethane	7.18	174	18088	11.24	ppb	97
60) MIBK (methyl isobutyl ket	8.13	43	35848	44.12	ppb	94
61) 1-Bromo-2-chloroethane	7.73	63	5895	9.31	ppb	91
63) Cis-1,3-Dichloropropene	7.93	75	16533	9.81	ppb #	91
64) Toluene	8.29	91	53393	10.12	ppb	94
65) Trans-1,3-Dichloropropene	8.56	75	16553	10.14	ppb	97
66) 1,1,2-TCA	8.75	97	11850	10.35	ppb	91
67) 2-Hexanone	9.06	43	25210	44.28	ppb	93
70) 1,2-EDB	9.28	107	14001	10.42	ppb #	90
71) Tetrachloroethene	8.90	166	30701	10.56	ppb	96
72) 1-Chlorohexane	9.85	91	17169	8.95	ppb	97
73) 1,1,1,2-Tetrachloroethane	9.94	131	22188	11.85	ppb	96
74) m&p-Xylene	10.11	91	105131	20.09	ppb	94
75) o-Xylene	10.54	91	53156	9.65	ppb	98
76) Styrene	10.56	104	41718	10.26	ppb	98
78) 1,3-Dichloropropane	8.93	76	17418	10.08	ppb	94
79) Dibromochloromethane	9.17	129	20697	11.19	ppb	98
80) Chlorobenzene	9.84	112	46068	10.03	ppb	100
81) Ethylbenzene	9.98	91	66757	9.81	ppb	99
82) Bromoform	10.74	173	19770	11.03	ppb	97
84) Isopropylbenzene	10.95	105	75818	9.77	ppb	94
85) 1,1,2,2-Tetrachloroethane	11.27	83	12422	8.06	ppb #	85
86) 1,2,3-Trichloropropane	11.31	110	6486	9.18	ppb	94
87) t-1,4-Dichloro-2-Butene	11.34	53	2838	8.09	ppb	95

(#) = qualifier out of range (m) = manual integration

Data File : M:\THOR\DATA\211111\1119T52.D  
 Acq On : 20 Nov 21 6:47  
 Sample : Ending CCV 10ug/L 11/19/21  
 Misc : IS&S 8/15/21

Vial: 52  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 22 11:04 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 10:21:13 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
88) Bromobenzene	11.26	156	28835	10.11	ppb	92
89) n-Propylbenzene	11.40	91	75253	8.80	ppb	100
90) 4-Ethyltoluene	11.53	105	72907	9.19	ppb	96
91) 2-Chlorotoluene	11.48	91	54389	9.34	ppb	94
92) 1,3,5-Trimethylbenzene	11.60	105	64367	9.10	ppb	97
93) 4-Chlorotoluene	11.60	91	55782	9.45	ppb	93
94) Tert-Butylbenzene	11.95	119	74359	10.10	ppb	96
95) 1,2,4-Trimethylbenzene	12.00	105	63930	9.49	ppb	99
96) Sec-Butylbenzene	12.19	105	79668	9.37	ppb	96
97) p-Isopropyltoluene	12.35	119	78369	9.73	ppb	94
98) Benzyl Chloride	12.55	91	20696	6.84	ppb	96
99) 1,3-DCB	12.30	146	50577	9.72	ppb	99
100) 1,4-DCB	12.40	146	50549	9.41	ppb	96
101) n-Butylbenzene	12.80	91	51068	9.01	ppb	98
102) 1,2-DCB	12.80	146	46649	9.81	ppb	96
103) Hexachloroethane	13.09	201	22858	10.69	ppb	90
104) 1,2-Dibromo-3-chloropropan	13.65	157	4847	8.28	ppb	94
105) 1,2,4-Trichlorobenzene	14.56	180	36341	9.45	ppb	94
106) Hexachlorobutadiene	14.76	225	26501	10.50	ppb	91
107) Naphthalene	14.83	128	24200	7.83	ppb	96
108) 1,2,3-Trichlorobenzene	15.09	180	33133	9.89	ppb	91

Quantitation Report


Data File : M:\THOR\DATA\211111\1119T52.D  
Acq On : 20 Nov 21 6:47  
Sample : Ending CCV 10ug/L 11/19/21  
Misc : IS&S 8/15/21

Vial: 52  
Operator:  
Inst : Thor  
Multiplr: 1.00

Quant Time: Nov 22 11:04 2021

Quant Results File: T1109W.RES

Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Wed Nov 10 10:21:13 2021  
Response via : Initial Calibration



VOLATILE ORGANIC ANALYSIS BY  
EPA METHOD 8260B

Form 7

Ending Continuing Calibration

Lab Name: APPL, Inc.

SDG No: \_\_\_\_\_

Case No: \_\_\_\_\_

Date Analyzed: 11/15/2021

Matrix: Water

Instrument: Max

Initial Cal. Date: 11/11/2021

Data File: 1115M25.D

		Compound	MEAN	CCRF	%D	%Drift
1	I	Fluorobenzene (IS)	ISTD			I
2	TM	Chlorotrifluoroethene	0.0000	0.0102	0.00	TM
3	TM	Dichlorodifluoromethane	0.1340	0.1318	1.7	TM
4	TM	Freon 114	0.0911	0.1008	11	TM
5	TM**L	Chloromethane	0.0872	0.0762	13	TM**L 2.7
6	TM*	Vinyl chloride	0.0927	0.0870	6.2	TM*
7	TM	2-Chloro-1,1,1-trifluoroethane	0.0000	0.0027	0.00	TM
8	TM	Bromomethane	0.1031	0.1041	0.90	TM
9	TML	Chloroethane	0.0887	0.0619	30	TML 0.72
10	TM	Dichlorofluoromethane	0.2076	0.2418	16	TM
11	TM	Trichlorofluoromethane	0.2656	0.3030	14	TM
12	TM	2,2-Dichloro-1,1,1-trifluoroethane	0.0000	0.0263	0.00	TM
13	TM	Acrolein	0.0117	0.0094	19	TM
14	TM	Acetone	0.0301	0.0294	2.2	TM
15	TM	Freon-113	0.1170	0.1363	17	TM
16	TM	Acetonitrile	0.0075	0.0069	8.8	TM
17	TML	2-propanol	0.0000	0.0006	0.00	TML
18	TM	1,2-Dichlorotrifluoroethane	0.2076	0.2418	16	TM
19	TM*L	1,1-DCE	0.1505	0.1738	16	TM*L 9.7
20	TM	t-Butanol	0.0104	0.0106	1.7	TM
21	TM	Methyl Acetate	0.0506	0.0511	1.00	TM
22	TML	Iodomethane	0.1104	0.1136	2.9	TML 13
23	TML	Acrylonitrile	0.0235	0.0304	29	TML 9.6
24	TML	2-Methylpentane	0.0000	0.0002	0.00	TML
25	TML	Methylene chloride	0.0919	0.1119	22	TML 11
26	TM	Carbon disulfide	0.1241	0.1308	5.4	TM
27	TML	Methyl t-butyl ether (MtBE)	0.3315	0.3809	15	TML 9.9
28	TM	Trans-1,2-DCE	0.1046	0.1220	17	TM
29	TML	3-Methylpentane	0.0636	0.0659	3.5	TML 14
30	TM	Hexane	0.0000	0.0001	0.00	TM
31	TM	Diisopropyl Ether	0.2118	0.2544	20	TM
32	TM**	1,1-DCA	0.1740	0.1852	6.5	TM**
33	TM	Ethyl tert Butyl Ether	0.2819	0.3234	15	TM
34	TML	Methylcyclopentane	0.0124	0.0123	0.87	TML 7.3
35	TM	MEK (2-Butanone)	0.0324	0.0344	6.2	TM
36	TML	Cis-1,2-DCE	0.1200	0.1280	6.6	TML 2.2
37	TM	2,2-Dichloropropane	0.2277	0.2194	3.7	TM
38	TM*	Chloroform	0.2428	0.2780	14	TM*
39	TML	Bromochloromethane	0.1009	0.1053	4.4	TML 3.9
40	S	Dibromofluoromethane(S)	0.3116	0.3248	4.2	S

Average

9.0

VOLATILE ORGANIC ANALYSIS BY  
EPA METHOD 8260B

Form 7

Ending Continuing Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Date Analyzed: 11/15/2021  
Instrument: Max  
Cal. Date: 11/11/2021  
Data File: 1115M25.D

		Compound	MEAN	CCRF	%D	%Drift
41	TML	1,1,1-TCA	0.2680	0.3212	20	TML 16
42	TML	Cyclohexane	0.0680	0.0779	15	TML 5.9
43	TM	1,1-Dichloropropene	0.1416	0.1609	14	TM
44	TM	2,2,4-Trimethylpentane	0.1982	0.1991	0.49	TM
45	S	1,2-DCA-D4(S)	0.2178	0.2285	4.9	S
46	TM	Carbon Tetrachloride	0.2554	0.2928	15	TM
47	TM	Tert Amyl Methyl Ether	0.2880	0.3215	12	TM
48	TM	1,2-DCA	0.2342	0.2591	11	TM
49	TM	Benzene	0.4057	0.4294	5.8	TM
50	TM	TCE	0.1300	0.1537	18	TM
51	TM	2-Pentanone	0.0533	0.0558	4.7	TM
52	TM*	1,2-Dichloropropane	0.0484	0.0456	5.9	TM*
53	TM	Bromodichloromethane	0.1904	0.2118	11	TM
54	TM	Methyl Cyclohexane	0.1466	0.1584	8.1	TM
55	TM	Dibromomethane	0.0784	0.0737	6.0	TM
56	TM	MIBK (methyl isobutyl ketone)	0.0662	0.0677	2.3	TM
57	TML	1-Bromo-2-chloroethane	0.0252	0.0288	14	TML 4.7
58	TML	2-Chloroethyl vinyl ether	0.0000	0.0001	0.00	TML
59	TM	Cis-1,3-Dichloropropene	0.1768	0.1903	7.6	TM
60	TM*	Toluene	0.5012	0.5154	2.8	TM*
61	TM	Trans-1,3-Dichloropropene	0.1693	0.1822	7.6	TM
62	TM	1,1,2-TCA	0.0736	0.0741	0.59	TM
63	TM	2-Hexanone	0.0431	0.0462	7.2	TM
64	I	Chlorobenzene-D5 (IS)	ISTD			I
65	S	Toluene-D8(S)	1.188	1.154	2.8	S
66	TM	1,2-EDB	0.1196	0.1313	9.7	TM
67	TML	Tetrachloroethene	0.1324	0.1306	1.3	TML 15
68	TM	1-Chlorohexane	0.0977	0.1043	6.8	TM
69	TM	1,1,1,2-Tetrachloroethane	0.2003	0.2016	0.63	TM
70	TM	m&p-Xylene	0.2709	0.2952	9.0	TM
71	TM	o-Xylene	0.2622	0.2824	7.7	TM
72	TM	Styrene	0.4145	0.4651	12	TM
73	S	4-Bromofluorobenzene(S)	0.4530	0.4645	2.5	S
74	TML	1,3-Dichloropropane	0.1649	0.1943	18	TML 10.0
75	TM	Dibromochloromethane	0.1925	0.2093	8.7	TM
76	TM**	Chlorobenzene	0.4034	0.4407	9.2	TM**
77	TM*	Ethylbenzene	0.6265	0.6965	11	TM*
78	TM**	Bromoform	0.1503	0.1668	11	TM**
79	I	1,4-Dichlorobenzene-D (IS)	ISTD			I
80	TM	Isopropylbenzene	1.066	1.168	9.6	TM

Average

8.3

VOLATILE ORGANIC ANALYSIS BY  
EPA METHOD 8260B

Form 7

Ending Continuing Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Date Analyzed: 11/15/2021  
Instrument: Max  
Cal. Date: 11/11/2021  
Data File: 1115M25.D

		Compound	MEAN	CCRF	%D	%Drift
81	TM**	1,1,2,2-Tetrachloroethane	0.1775	0.1679	5.4	TM**
82	TML	1,2,3-Trichloropropane	0.1011	0.1086	7.5	TML 20
83	TML	t-1,4-Dichloro-2-Butene	0.0414	0.0491	19	TML 15
84	TM	Bromobenzene	0.3809	0.3948	3.6	TM
85	TM	n-Propylbenzene	1.042	1.183	14	TM
86	TM	4-Ethyltoluene	1.021	1.119	9.6	TM
87	TM	2-Chlorotoluene	0.8206	0.9040	10	TM
88	TM	1,3,5-Trimethylbenzene	0.9005	1.022	13	TM
89	TM	4-Chlorotoluene	0.8292	0.9488	14	TM
90	TM	Tert-Butylbenzene	0.5251	0.6078	16	TM
91	TM	1,2,4-Trimethylbenzene	0.8840	0.9587	8.5	TM
92	TM	Sec-Butylbenzene	0.9755	1.173	20	TM
93	TML	p-Isopropyltoluene	0.9027	1.066	18	TML 3.2
94	TML	Benzyl Chloride	0.2431	0.2068	15	TML 8.1
95	TM	1,3-DCB	0.6521	0.6594	1.1	TM
96	TM	1,4-DCB	0.6758	0.6388	5.5	TM
97	TML	n-Butylbenzene	0.5559	0.5788	4.1	TML 9.4
98	TM	1,2-DCB	0.6054	0.6610	9.2	TM
99	TML	Hexachloroethane	0.1637	0.1983	21	TML 12
100	TML	1,2-Dibromo-3-chloropropane	0.0435	0.0528	21	TML 6.8
101	TML	1,2,4-Trichlorobenzene	0.1844	0.2147	16	TML 9.5
102	TML	Hexachlorobutadiene	0.2201	0.2648	20	TML 2.5
103	TML	Naphthalene	0.3408	0.3262	4.2	TML 17
104	TML	1,2,3-Trichlorobenzene	0.2270	0.2524	11	TML 14
105						
106						
107						
108						
109						
110						
111						
112						
113						
114						
115						
116						
117						
118						
119						
120						

Average

11.9



Data File : M:\MAX\DATA\211111\1115M25.D  
 Acq On : 15 Nov 21 19:52  
 Sample : Ending CCV 10ug/L 11/15/21  
 Misc : IS&S 8/4/21

Vial: 25  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 16 4:12 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:40:33 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.37	96	380344	25.00	ppb	0.00
65) Chlorobenzene-D5 (IS)	9.53	117	342457	25.00	ppb	0.00
80) 1,4-Dichlorobenzene-D (IS)	11.85	152	222128	25.00	ppb	0.00

System Monitoring Compounds

41) Dibromofluoromethane(S)	5.59	111	123534	26.06	ppb	0.00
Spiked Amount	25.000		Recovery	=	104.232%	
46) 1,2-DCA-D4(S)	5.98	65	86896	26.23	ppb	0.00
Spiked Amount	25.000		Recovery	=	104.920%	
66) Toluene-D8(S)	8.08	98	395285	24.29	ppb	0.00
Spiked Amount	25.000		Recovery	=	97.168%	
74) 4-Bromofluorobenzene(S)	10.70	95	159067	25.63	ppb	0.00
Spiked Amount	25.000		Recovery	=	102.532%	

Target Compounds

	R.T.	QIon	Response	Conc	Units	Qvalue
3) Dichlorodifluoromethane	1.20	85	20048	9.83	ppb	95
4) Freon 114	1.30	85	15329	11.06	ppb	94
5) Chloromethane	1.34	50	11591	9.73	ppb	98
6) Vinyl chloride	1.43	62	13234	9.38	ppb	92
8) Bromomethane	1.69	94	15833	10.09	ppb	98
9) Chloroethane	1.79	64	9417	10.07	ppb	96
10) Dichlorofluoromethane	1.99	67	36785	11.65	ppb	97
11) Trichlorofluoromethane	2.02	101	46095	11.41	ppb	98
13) Acrolein	2.46	56	17946	101.14	ppb	93
14) Acetone	2.63	43	22377	48.88	ppb	96
15) Freon-113	2.55	151	20740	11.65	ppb	93
16) Acetonitrile	2.96	41	13041	113.94	ppb	95
18) 1,2-Dichlorotrifluoroethan	1.99	67	36785	11.65	ppb	100
19) 1,1-DCE	2.53	61	26442	10.97	ppb	99
20) t-Butanol	3.37	59	20172	127.09	ppb	99
21) Methyl Acetate	3.02	43	7779	10.10	ppb	98
22) Iodomethane	2.68	142	17281	8.70	ppb	95
23) Acrylonitrile	3.46	53	4622	10.96	ppb	96
25) Methylene chloride	3.11	84	17023	11.12	ppb	90
26) Carbon disulfide	2.74	76	19896	10.54	ppb	97
27) Methyl t-butyl ether (MtBE)	3.50	73	57951	10.99	ppb	98
28) Trans-1,2-DCE	3.46	96	18558	11.66	ppb	82
29) 3-Methylpentane	3.50	57	10019	11.45	ppb	84
31) Diisopropyl Ether	4.28	45	38707	12.01	ppb	91
32) 1,1-DCA	4.10	63	28176	10.65	ppb	96
34) Ethyl tert Butyl Ether	4.81	59	49200	11.47	ppb	91
35) Methylcyclopentane	4.81	56	1866	9.27	ppb	100

(#) = qualifier out of range (m) = manual integration

Data File : M:\MAX\DATA\211111\1115M25.D  
 Acq On : 15 Nov 21 19:52  
 Sample : Ending CCV 10ug/L 11/15/21  
 Misc : IS&S 8/4/21

Vial: 25  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 16 4:12 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:40:33 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
36) MEK (2-Butanone)	5.03	43	26203	53.12	ppb	# 91
37) Cis-1,2-DCE	4.95	96	19474	10.22	ppb	93
38) 2,2-Dichloropropane	4.93	77	33382	9.63	ppb	96
39) Chloroform	5.39	83	42292	11.45	ppb	84
40) Bromochloromethane	5.26	130	16013	10.39	ppb	87
42) 1,1,1-TCA	5.57	97	48866	11.64	ppb	93
43) Cyclohexane	5.62	41	11847	10.59	ppb	85
44) 1,1-Dichloropropene	5.79	75	24483	11.37	ppb	88
45) 2,2,4-Trimethylpentane	6.15	57	30296	10.05	ppb	95
47) Carbon Tetrachloride	5.77	117	44552	11.47	ppb	87
48) Tert Amyl Methyl Ether	6.21	73	48907	11.16	ppb	# 94
49) 1,2-DCA	6.07	62	39413	11.06	ppb	98
50) Benzene	6.03	78	65334	10.58	ppb	94
51) TCE	6.78	95	23386	11.82	ppb	98
52) 2-Pentanone	7.04	43	106087	130.83	ppb	95
53) 1,2-Dichloropropane	7.03	63	6930	9.41	ppb	97
54) Bromodichloromethane	7.34	83	32219	11.12	ppb	100
55) Methyl Cyclohexane	6.97	83	24103	10.81	ppb	96
56) Dibromomethane	7.15	93	11218	9.40	ppb	78
57) MIBK (methyl isobutyl ket	8.01	43	51530	51.16	ppb	94
58) 1-Bromo-2-chloroethane	7.65	144	4381	10.47	ppb	84
60) Cis-1,3-Dichloropropene	7.82	75	28945	10.76	ppb	91
61) Toluene	8.14	91	78408	10.28	ppb	90
62) Trans-1,3-Dichloropropene	8.40	75	27717	10.76	ppb	97
63) 1,1,2-TCA	8.58	83	11269	10.06	ppb	93
64) 2-Hexanone	8.85	43	35157	53.60	ppb	94
67) 1,2-EDB	9.06	107	17981	10.97	ppb	90
68) Tetrachloroethene	8.69	164	17896	11.48	ppb	92
69) 1-Chlorohexane	9.56	91	14286	10.68	ppb	94
70) 1,1,1,2-Tetrachloroethane	9.65	131	27610	10.06	ppb	90
71) m&p-Xylene	9.79	106	80866	21.79	ppb	98
72) o-Xylene	10.19	106	38686	10.77	ppb	94
73) Styrene	10.20	104	63710	11.22	ppb	97
75) 1,3-Dichloropropane	8.74	76	26617	11.00	ppb	94
76) Dibromochloromethane	8.96	129	28670	10.87	ppb	81
77) Chlorobenzene	9.55	112	60367	10.92	ppb	92
78) Ethylbenzene	9.68	91	95402	11.12	ppb	96
79) Bromoform	10.37	173	22852	11.10	ppb	97
81) Isopropylbenzene	10.56	105	103735	10.96	ppb	98
82) 1,1,2,2-Tetrachloroethane	10.87	83	14915	9.46	ppb	# 90
83) 1,2,3-Trichloropropane	10.90	110	9653	11.98	ppb	99
84) t-1,4-Dichloro-2-Butene	10.93	53	4366	11.55	ppb	87

(#) = qualifier out of range (m) = manual integration

Data File : M:\MAX\DATA\211111\1115M25.D  
 Acq On : 15 Nov 21 19:52  
 Sample : Ending CCV 10ug/L 11/15/21  
 Misc : IS&S 8/4/21

Vial: 25  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 16 4:12 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:40:33 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
85) Bromobenzene	10.84	156	35077	10.36	ppb	75
86) n-Propylbenzene	10.97	91	105102	11.35	ppb	96
87) 4-Ethyltoluene	11.08	105	99444	10.96	ppb	95
88) 2-Chlorotoluene	11.04	91	80324	11.02	ppb	98
89) 1,3,5-Trimethylbenzene	11.15	105	90785	11.35	ppb	99
90) 4-Chlorotoluene	11.15	91	84298	11.44	ppb	92
91) Tert-Butylbenzene	11.47	119	54000	11.57	ppb	97
92) 1,2,4-Trimethylbenzene	11.51	105	85183	10.85	ppb	93
93) Sec-Butylbenzene	11.68	105	104235	12.03	ppb	95
94) p-Isopropyltoluene	11.83	119	94704	10.32	ppb	96
95) Benzyl Chloride	12.01	91	18377	9.19	ppb	# 92
96) 1,3-DCB	11.78	146	58586	10.11	ppb	97
97) 1,4-DCB	11.87	146	56755	9.45	ppb	94
98) n-Butylbenzene	12.24	91	51430	9.06	ppb	99
99) 1,2-DCB	12.24	146	58728	10.92	ppb	95
100) Hexachloroethane	12.48	117	17619	11.22	ppb	81
101) 1,2-Dibromo-3-chloropropan	13.02	75	4694	10.68	ppb	92
102) 1,2,4-Trichlorobenzene	13.84	180	19072	9.05	ppb	98
103) Hexachlorobutadiene	14.01	225	23524	9.75	ppb	92
104) Naphthalene	14.08	128	28982	8.35	ppb	# 91
105) 1,2,3-Trichlorobenzene	14.32	180	22429	8.65	ppb	98

(#) = qualifier out of range (m) = manual integration


Data File : M:\MAX\DATA\211111\1115M25.D  
Acq On : 15 Nov 21 19:52  
Sample : Ending CCV 10ug/L 11/15/21  
Misc : IS&S 8/4/21

Vial: 25  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Nov 16 4:12 2021

Quant Results File: M1111W.RES

Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Fri Nov 12 09:40:33 2021  
Response via : Initial Calibration



Data File : M:\MAX\DATA\211111\1115M12.D  
 Acq On : 15 Nov 21 13:44  
 Sample : BA46114W01  
 Misc : IS&S 8/4/21

Vial: 12  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 16 4:51 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:40:33 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.38	96	363931	25.00	ppb	0.00
65) Chlorobenzene-D5 (IS)	9.53	117	329377	25.00	ppb	0.00
80) 1,4-Dichlorobenzene-D (IS)	11.85	152	206728	25.00	ppb	0.00
System Monitoring Compounds						
41) Dibromofluoromethane(S)	5.60	111	120212	26.50	ppb	0.00
Spiked Amount	25.000		Recovery	=	106.004%	
46) 1,2-DCA-D4(S)	5.98	65	82336	25.97	ppb	0.00
Spiked Amount	25.000		Recovery	=	103.900%	
66) Toluene-D8(S)	8.08	98	383891	24.53	ppb	0.00
Spiked Amount	25.000		Recovery	=	98.112%	
74) 4-Bromofluorobenzene(S)	10.71	95	150594	25.23	ppb	0.00
Spiked Amount	25.000		Recovery	=	100.928%	

Target Compounds

Qvalue

Quantitation Report


Data File : M:\MAX\DATA\211111\1115M12.D  
Acq On : 15 Nov 21 13:44  
Sample : BA46114W01  
Misc : IS&S 8/4/21

Vial: 12  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Nov 16 4:51 2021

Quant Results File: M1111W.RES

Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Fri Nov 12 09:40:33 2021  
Response via : Initial Calibration



Data File : M:\MAX\DATA\211111\1115M13.D  
 Acq On : 15 Nov 21 14:12  
 Sample : BA46115W01  
 Misc : IS&S 8/4/21

Vial: 13  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 16 4:54 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:40:33 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.38	96	382634	25.00	ppb	0.00
65) Chlorobenzene-D5 (IS)	9.53	117	339368	25.00	ppb	0.00
80) 1,4-Dichlorobenzene-D (IS)	11.85	152	200988	25.00	ppb	0.00
System Monitoring Compounds						
41) Dibromofluoromethane(S)	5.60	111	127338	26.70	ppb	0.00
Spiked Amount	25.000		Recovery	=	106.800%	
46) 1,2-DCA-D4(S)	5.99	65	86592	25.98	ppb	0.00
Spiked Amount	25.000		Recovery	=	103.928%	
66) Toluene-D8(S)	8.08	98	401175	24.88	ppb	0.00
Spiked Amount	25.000		Recovery	=	99.512%	
74) 4-Bromofluorobenzene(S)	10.71	95	151857	24.69	ppb	0.00
Spiked Amount	25.000		Recovery	=	98.776%	

Target Compounds

Qvalue

Quantitation Report


Data File : M:\MAX\DATA\211111\1115M13.D  
Acq On : 15 Nov 21 14:12  
Sample : BA46115W01  
Misc : IS&S 8/4/21

Vial: 13  
Operator: LP, DG, CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Nov 16 4:54 2021

Quant Results File: M1111W.RES

Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Fri Nov 12 09:40:33 2021  
Response via : Initial Calibration





Data File : M:\MAX\DATA\211111\1115M14.D  
 Acq On : 15 Nov 21 14:40  
 Sample : BA46116W01  
 Misc : IS&S 8/4/21

Vial: 14  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 16 4:55 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:40:33 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.38	96	376769	25.00	ppb	0.00
65) Chlorobenzene-D5 (IS)	9.53	117	341407	25.00	ppb	0.00
80) 1,4-Dichlorobenzene-D (IS)	11.85	152	199848	25.00	ppb	0.00
System Monitoring Compounds						
41) Dibromofluoromethane (S)	5.60	111	125188	26.66	ppb	0.00
Spiked Amount						
						Recovery = 106.632%
46) 1,2-DCA-D4 (S)	5.98	65	84968	25.89	ppb	0.00
Spiked Amount						
						Recovery = 103.568%
66) Toluene-D8 (S)	8.08	98	382728	23.59	ppb	0.00
Spiked Amount						
						Recovery = 94.368%
74) 4-Bromofluorobenzene (S)	10.71	95	147342	23.82	ppb	0.00
Spiked Amount						
						Recovery = 95.268%

Target Compounds Qvalue

Quantitation Report


Data File : M:\MAX\DATA\211111\1115M14.D  
Acq On : 15 Nov 21 14:40  
Sample : BA46116W01  
Misc : IS&S 8/4/21

Vial: 14  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Nov 16 4:55 2021

Quant Results File: M1111W.RES

Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Fri Nov 12 09:40:33 2021  
Response via : Initial Calibration



**ORGANICS**  
**Raw Data**

Data File : M:\MAX\DATA\211111\1115M12.D  
 Acq On : 15 Nov 21 13:44  
 Sample : BA46114W01  
 Misc : IS&S 8/4/21

Vial: 12  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 16 4:51 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:40:33 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.38	96	363931	25.00	ppb	0.00
65) Chlorobenzene-D5 (IS)	9.53	117	329377	25.00	ppb	0.00
80) 1,4-Dichlorobenzene-D (IS)	11.85	152	206728	25.00	ppb	0.00
System Monitoring Compounds						
41) Dibromofluoromethane(S)	5.60	111	120212	26.50	ppb	0.00
Spiked Amount	25.000		Recovery	=	106.004%	
46) 1,2-DCA-D4(S)	5.98	65	82336	25.97	ppb	0.00
Spiked Amount	25.000		Recovery	=	103.900%	
66) Toluene-D8(S)	8.08	98	383891	24.53	ppb	0.00
Spiked Amount	25.000		Recovery	=	98.112%	
74) 4-Bromofluorobenzene(S)	10.71	95	150594	25.23	ppb	0.00
Spiked Amount	25.000		Recovery	=	100.928%	

Target Compounds Qvalue

Quantitation Report


Data File : M:\MAX\DATA\211111\1115M12.D  
Acq On : 15 Nov 21 13:44  
Sample : BA46114W01  
Misc : IS&S 8/4/21

Vial: 12  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Nov 16 4:51 2021

Quant Results File: M1111W.RES

Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Fri Nov 12 09:40:33 2021  
Response via : Initial Calibration



Data File : M:\MAX\DATA\211111\1115M13.D  
 Acq On : 15 Nov 21 14:12  
 Sample : BA46115W01  
 Misc : IS&S 8/4/21

Vial: 13  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 16 4:54 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:40:33 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.38	96	382634	25.00	ppb	0.00
65) Chlorobenzene-D5 (IS)	9.53	117	339368	25.00	ppb	0.00
80) 1,4-Dichlorobenzene-D (IS)	11.85	152	200988	25.00	ppb	0.00
System Monitoring Compounds						
41) Dibromofluoromethane(S)	5.60	111	127338	26.70	ppb	0.00
Spiked Amount						
						Recovery = 106.800%
46) 1,2-DCA-D4(S)	5.99	65	86592	25.98	ppb	0.00
Spiked Amount						
						Recovery = 103.928%
66) Toluene-D8(S)	8.08	98	401175	24.88	ppb	0.00
Spiked Amount						
						Recovery = 99.512%
74) 4-Bromofluorobenzene(S)	10.71	95	151857	24.69	ppb	0.00
Spiked Amount						
						Recovery = 98.776%

Target Compounds

Qvalue

Quantitation Report


Data File : M:\MAX\DATA\211111\1115M13.D  
Acq On : 15 Nov 21 14:12  
Sample : BA46115W01  
Misc : IS&S 8/4/21

Vial: 13  
Operator: LP, DG, CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Nov 16 4:54 2021

Quant Results File: M1111W.RES

Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Fri Nov 12 09:40:33 2021  
Response via : Initial Calibration



Data File : M:\MAX\DATA\211111\1115M14.D  
 Acq On : 15 Nov 21 14:40  
 Sample : BA46116W01  
 Misc : IS&S 8/4/21

Vial: 14  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 16 4:55 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:40:33 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.38	96	376769	25.00	ppb	0.00
65) Chlorobenzene-D5 (IS)	9.53	117	341407	25.00	ppb	0.00
80) 1,4-Dichlorobenzene-D (IS)	11.85	152	199848	25.00	ppb	0.00
<b>System Monitoring Compounds</b>						
41) Dibromofluoromethane(S)	5.60	111	125188	26.66	ppb	0.00
Spiked Amount				25.000		
						Recovery = 106.632%
46) 1,2-DCA-D4(S)	5.98	65	84968	25.89	ppb	0.00
Spiked Amount				25.000		
						Recovery = 103.568%
66) Toluene-D8(S)	8.08	98	382728	23.59	ppb	0.00
Spiked Amount				25.000		
						Recovery = 94.368%
74) 4-Bromofluorobenzene(S)	10.71	95	147342	23.82	ppb	0.00
Spiked Amount				25.000		
						Recovery = 95.268%

Target Compounds Qvalue



Quantitation Report


Data File : M:\MAX\DATA\211111\1115M14.D  
Acq On : 15 Nov 21 14:40  
Sample : BA46116W01  
Misc : IS&S 8/4/21

Vial: 14  
Operator: LP, DG, CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Nov 16 4:55 2021

Quant Results File: M1111W.RES

Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Fri Nov 12 09:40:33 2021  
Response via : Initial Calibration



Data File : M:\MAX\DATA\211111\1115M08.D  
 Acq On : 15 Nov 21 11:50  
 Sample : 211115A BLK  
 Misc : IS&S 8/4/21

Vial: 8  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 15 12:51 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:40:33 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.38	96	395694	25.00	ppb	0.00
65) Chlorobenzene-D5 (IS)	9.53	117	350184	25.00	ppb	0.00
80) 1,4-Dichlorobenzene-D (IS)	11.85	152	211146	25.00	ppb	0.00
System Monitoring Compounds						
41) Dibromofluoromethane(S)	5.60	111	126243	25.60	ppb	0.00
Spiked Amount	25.000		Recovery	=	102.388%	
46) 1,2-DCA-D4(S)	5.98	65	84272	24.45	ppb	0.00
Spiked Amount	25.000		Recovery	=	97.804%	
66) Toluene-D8(S)	8.08	98	406449	24.43	ppb	0.00
Spiked Amount	25.000		Recovery	=	97.708%	
74) 4-Bromofluorobenzene(S)	10.71	95	157554	24.83	ppb	0.00
Spiked Amount	25.000		Recovery	=	99.316%	

Target Compounds

Qvalue

(#) = qualifier out of range (m) = manual integration


Data File : M:\MAX\DATA\211111\1115M08.D  
Acq On : 15 Nov 21 11:50  
Sample : 211115A BLK  
Misc : IS&S 8/4/21

Vial: 8  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Nov 15 12:51 2021

Quant Results File: M1111W.RES

Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Fri Nov 12 09:40:33 2021  
Response via : Initial Calibration



Data File : M:\THOR\DATA\211111\1119T37.D  
 Acq On : 20 Nov 21 00:39  
 Sample : 211119B BLK  
 Misc : IS&S 8/15/21

Vial: 37  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 22 11:25 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 10:21:13 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.35	96	253564	25.00	ppb	0.00
68) Chlorobenzene-D5 (IS)	9.81	117	256153	25.00	ppb	0.00
83) 1,4-Dichlorobenzene-D (IS)	12.37	152	187736	25.00	ppb	0.00
System Monitoring Compounds						
43) Dibromofluoromethane(S)	5.50	111	80071	28.22	ppb	0.00
Spiked Amount	25.000		Recovery	=	112.884%	
48) 1,2-DCA-D4(S)	5.91	65	88040	28.99	ppb	0.00
Spiked Amount	25.000		Recovery	=	115.956%	
69) Toluene-D8(S)	8.22	98	260114	25.82	ppb	0.00
Spiked Amount	25.000		Recovery	=	103.284%	
77) 4-Bromofluorobenzene(S)	11.11	95	102793	25.57	ppb	0.00
Spiked Amount	25.000		Recovery	=	102.272%	

Target Compounds

Qvalue

Quantitation Report


Data File : M:\THOR\DATA\211111\1119T37.D  
Acq On : 20 Nov 21 00:39  
Sample : 211119B BLK  
Misc : IS&S 8/15/21

Vial: 37  
Operator:  
Inst : Thor  
Multiplr: 1.00

Quant Time: Nov 22 11:25 2021

Quant Results File: T1109W.RES

Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Wed Nov 10 10:21:13 2021  
Response via : Initial Calibration



Data File : M:\MAX\DATA\211111\1115M04.D Vial: 4  
 Acq On : 15 Nov 21 9:57 Operator: LP,DG,CH  
 Sample : 211115A LCSD 10ug/L Inst : Max  
 Misc : IS&S 8/4/21 Multiplr: 1.00

Quant Time: Nov 16 5:34 2021 Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:40:33 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.38	96	411326	25.00	ppb	0.00
65) Chlorobenzene-D5 (IS)	9.53	117	355924	25.00	ppb	0.00
80) 1,4-Dichlorobenzene-D (IS)	11.85	152	229762	25.00	ppb	0.00

System Monitoring Compounds

41) Dibromofluoromethane(S)	5.60	111	127171	24.80	ppb	0.00
Spiked Amount	25.000		Recovery	=	99.220%	
46) 1,2-DCA-D4(S)	5.99	65	87856	24.52	ppb	0.00
Spiked Amount	25.000		Recovery	=	98.092%	
66) Toluene-D8(S)	8.08	98	420129	24.84	ppb	0.00
Spiked Amount	25.000		Recovery	=	99.368%	
74) 4-Bromofluorobenzene(S)	10.71	95	160621	24.90	ppb	0.00
Spiked Amount	25.000		Recovery	=	99.616%	

Target Compounds

	R.T.	QIon	Response	Conc	Units	Qvalue
3) Dichlorodifluoromethane	1.20	85	20192	9.16	ppb	96
4) Freon 114	1.30	85	13544	9.04	ppb	84
5) Chloromethane	1.34	50	12322	9.56	ppb	94
6) Vinyl chloride	1.43	62	14289	9.37	ppb	84
8) Bromomethane	1.70	94	13865	8.17	ppb	96
9) Chloroethane	1.79	64	9536	9.36	ppb	88
10) Dichlorofluoromethane	1.99	67	33806	9.90	ppb	96
11) Trichlorofluoromethane	2.03	101	43270	9.90	ppb	96
13) Acrolein	2.46	56	23216	120.98	ppb	82
14) Acetone	2.64	43	21544	43.52	ppb	94
15) Freon-113	2.55	151	18206	9.46	ppb	# 86
16) Acetonitrile	2.96	41	13351	107.86	ppb	# 86
18) 1,2-Dichlorotrifluoroethan	1.99	67	33806	9.90	ppb	100
19) 1,1-DCE	2.54	61	24689	9.48	ppb	98
20) t-Butanol	3.37	59	19264	112.23	ppb	# 91
21) Methyl Acetate	3.03	43	6476	7.77	ppb	# 79
22) Iodomethane	2.69	142	19595	9.07	ppb	89
23) Acrylonitrile	3.47	53	5293	11.61	ppb	# 82
25) Methylene chloride	3.12	84	15802	9.53	ppb	# 92
26) Carbon disulfide	2.74	76	19272	9.44	ppb	94
27) Methyl t-butyl ether (MtBE)	3.51	73	58390	10.20	ppb	96
28) Trans-1,2-DCE	3.48	96	16940	9.84	ppb	96
29) 3-Methylpentane	3.51	57	9799	10.30	ppb	# 98
31) Diisopropyl Ether	4.28	45	36935	10.60	ppb	94
32) 1,1-DCA	4.11	63	29548	10.32	ppb	95
34) Ethyl tert Butyl Ether	4.81	59	46950	10.12	ppb	98
35) Methylcyclopentane	4.82	56	2207	10.38	ppb	100

(#) = qualifier out of range (m) = manual integration

Data File : M:\MAX\DATA\211111\1115M04.D  
 Acq On : 15 Nov 21 9:57  
 Sample : 211115A LCSD 10ug/L  
 Misc : IS&S 8/4/21

Vial: 4  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 16 5:34 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:40:33 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
36) MEK (2-Butanone)	5.03	43	25615	48.02	ppb	95
37) Cis-1,2-DCE	4.95	96	19987	9.68	ppb	94
38) 2,2-Dichloropropane	4.94	77	40662	10.85	ppb	96
39) Chloroform	5.40	83	40570	10.16	ppb	89
40) Bromochloromethane	5.26	130	16775	10.05	ppb	92
42) 1,1,1-TCA	5.58	97	46813	10.26	ppb	94
43) Cyclohexane	5.63	41	11697	9.65	ppb	79
44) 1,1-Dichloropropene	5.79	75	22640	9.72	ppb	94
45) 2,2,4-Trimethylpentane	6.15	57	30536	9.37	ppb	94
47) Carbon Tetrachloride	5.78	117	41523	9.88	ppb	91
48) Tert Amyl Methyl Ether	6.22	73	46954	9.91	ppb	97
49) 1,2-DCA	6.08	62	35139	9.12	ppb	95
50) Benzene	6.03	78	64351	9.64	ppb	96
51) TCE	6.79	95	19814	9.26	ppb	93
52) 2-Pentanone	7.04	43	109714	125.11	ppb	100
53) 1,2-Dichloropropane	7.03	63	7287	9.15	ppb #	87
54) Bromodichloromethane	7.35	83	31828	10.16	ppb	99
55) Methyl Cyclohexane	6.98	83	22644	9.39	ppb	97
56) Dibromomethane	7.16	93	11278	8.74	ppb	91
57) MIBK (methyl isobutyl ket	8.01	43	55476	50.93	ppb	96
58) 1-Bromo-2-chloroethane	7.66	144	3901	8.58	ppb	80
60) Cis-1,3-Dichloropropene	7.82	75	27736	9.53	ppb	92
61) Toluene	8.15	91	77248	9.37	ppb	92
62) Trans-1,3-Dichloropropene	8.40	75	27307	9.80	ppb	96
63) 1,1,2-TCA	8.58	83	11847	9.78	ppb	97
64) 2-Hexanone	8.86	43	34274	48.31	ppb	90
67) 1,2-EDB	9.06	107	17374	10.20	ppb	95
68) Tetrachloroethene	8.70	164	16355	10.03	ppb	94
69) 1-Chlorohexane	9.56	91	14349	10.32	ppb	95
70) 1,1,1,2-Tetrachloroethane	9.65	131	27916	9.79	ppb	96
71) m&p-Xylene	9.80	106	76153	19.75	ppb	95
72) o-Xylene	10.19	106	38054	10.20	ppb	99
73) Styrene	10.21	104	62385	10.57	ppb	95
75) 1,3-Dichloropropane	8.74	76	25089	9.95	ppb	89
76) Dibromochloromethane	8.97	129	28663	10.46	ppb	97
77) Chlorobenzene	9.56	112	60130	10.47	ppb	92
78) Ethylbenzene	9.68	91	93078	10.44	ppb	100
79) Bromoform	10.38	173	23117	10.80	ppb	91
81) Isopropylbenzene	10.56	105	96164	9.82	ppb	99
82) 1,1,2,2-Tetrachloroethane	10.87	83	16078	9.86	ppb #	88
83) 1,2,3-Trichloropropane	10.90	110	8650	10.33	ppb	95
84) t-1,4-Dichloro-2-Butene	10.94	53	4658	11.90	ppb	97

(#) = qualifier out of range (m) = manual integration  
 1115M04.D M1111W.M Tue Nov 16 08:00:02 2021

Data File : M:\MAX\DATA\211111\1115M04.D  
 Acq On : 15 Nov 21 9:57  
 Sample : 211115A LCSD 10ug/L  
 Misc : IS&S 8/4/21

Vial: 4  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 16 5:34 2021

Quant Results File: M1111W.RES

Quant Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Fri Nov 12 09:40:33 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
85) Bromobenzene	10.84	156	34200	9.77	ppb	90
86) n-Propylbenzene	10.97	91	101561	10.60	ppb	95
87) 4-Ethyltoluene	11.09	105	96466	10.28	ppb	99
88) 2-Chlorotoluene	11.04	91	79701	10.57	ppb	99
89) 1,3,5-Trimethylbenzene	11.15	105	89917	10.86	ppb	95
90) 4-Chlorotoluene	11.15	91	79116	10.38	ppb	90
91) Tert-Butylbenzene	11.47	119	51144	10.60	ppb	98
92) 1,2,4-Trimethylbenzene	11.52	105	85691	10.55	ppb	96
93) Sec-Butylbenzene	11.69	105	98644	11.00	ppb	97
94) p-Isopropyltoluene	11.84	119	91971	9.73	ppb	98
95) Benzyl Chloride	12.02	91	24273	11.38	ppb	93
96) 1,3-DCB	11.78	146	59603	9.94	ppb	98
97) 1,4-DCB	11.87	146	60501	9.74	ppb	96
98) n-Butylbenzene	12.24	91	52671	8.99	ppb	96
99) 1,2-DCB	12.24	146	55620	10.00	ppb	99
100) Hexachloroethane	12.49	117	15225	9.47	ppb	98
101) 1,2-Dibromo-3-chloropropan	13.02	75	4221	9.42	ppb	94
102) 1,2,4-Trichlorobenzene	13.84	180	17760	8.38	ppb	97
103) Hexachlorobutadiene	14.02	225	23311	9.39	ppb	98
104) Naphthalene	14.08	128	30634	8.46	ppb	97
105) 1,2,3-Trichlorobenzene	14.32	180	22260	8.40	ppb	94

(#) = qualifier out of range (m) = manual integration

1115M04.D M1111W.M Tue Nov 16 08:00:02 2021

Page 3




Data File : M:\MAX\DATA\211111\1115M04.D  
Acq On : 15 Nov 21 9:57  
Sample : 211115A LCSD 10ug/L  
Misc : IS&S 8/4/21

Vial: 4  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Nov 16 5:34 2021

Quant Results File: M1111W.RES

Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Fri Nov 12 09:40:33 2021  
Response via : Initial Calibration



Data File : M:\THOR\DATA\211111\1119T32.D  
 Acq On : 19 Nov 21 22:36  
 Sample : 211119B LCSD 10ug/L  
 Misc : IS&S 8/15/21

Vial: 32  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 22 11:04 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 10:21:13 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.34	96	256465	25.00	ppb	0.00
68) Chlorobenzene-D5 (IS)	9.81	117	260381	25.00	ppb	0.00
83) 1,4-Dichlorobenzene-D (IS)	12.37	152	196706	25.00	ppb	0.00
System Monitoring Compounds						
43) Dibromofluoromethane(S)	5.49	111	82167	28.63	ppb	0.00
Spiked Amount				25.000		
				Recovery	=	114.528%
48) 1,2-DCA-D4(S)	5.91	65	87283	28.41	ppb	0.00
Spiked Amount				25.000		
				Recovery	=	113.656%
69) Toluene-D8(S)	8.22	98	262306	25.62	ppb	0.00
Spiked Amount				25.000		
				Recovery	=	102.464%
77) 4-Bromofluorobenzene(S)	11.11	95	108427	26.53	ppb	0.00
Spiked Amount				25.000		
				Recovery	=	106.124%
Target Compounds						Qvalue
3) Dichlorodifluoromethane	1.09	85	6639	8.27	ppb	90
4) Freon 114	1.20	85	7523	11.00	ppb	99
5) Chloromethane	1.27	50	2639	9.53	ppb	92
6) Vinyl chloride	1.32	62	5827	8.23	ppb	98
9) Bromomethane	1.59	96	5795	10.38	ppb	97
10) Chloroethane	1.68	64	3851	10.20	ppb	93
11) Dichlorofluoromethane	1.86	67	16411	11.15	ppb	97
12) Trichlorofluoromethane	1.91	101	26472	10.85	ppb	98
16) Acrolein	2.31	56	6499	51.12	ppb	88
17) Acetone	2.47	43	11624	48.24	ppb	95
18) Freon-113	2.43	101	5708	9.80	ppb	99
19) 1,1-DCE	2.41	61	13676	9.28	ppb	92
21) Acetonitrile	2.79	40	1086	84.81	ppb	# 91
22) t-Butanol	3.16	59	3809	117.73	ppb	95
23) Methyl Acetate	2.87	43	4450	9.52	ppb	# 84
24) Iodomethane	2.55	142	4920	8.69	ppb	97
25) Acrylonitrile	3.30	52	1379	8.75	ppb	# 63
26) Methylene chloride	2.96	49	8649	9.15	ppb	# 80
27) Carbon disulfide	2.61	76	8949	7.58	ppb	98
28) Methyl t-butyl ether (MtBE)	3.33	73	30068	11.17	ppb	96
29) Trans-1,2-DCE	3.31	61	11171	8.92	ppb	91
31) Diisopropyl Ether	4.12	45	17524	9.06	ppb	99
33) 1,1-DCA	3.92	63	14779	9.44	ppb	97
34) Vinyl Acetate	4.11	43	13424	8.19	ppb	98
35) Ethyl tert Butyl Ether	4.67	59	25653	11.06	ppb	92
36) MEK (2-Butanone)	4.87	43	14371	46.44	ppb	99
37) Cis-1,2-DCE	4.81	61	14023	10.41	ppb	96

(#) = qualifier out of range (m) = manual integration

Data File : M:\THOR\DATA\211111\1119T32.D  
 Acq On : 19 Nov 21 22:36  
 Sample : 211119B LCSD 10ug/L  
 Misc : IS&S 8/15/21

Vial: 32  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 22 11:04 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 10:21:13 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
38) 2,2-Dichloropropane	4.79	77	20606	11.69	ppb	99
40) 3-Methylpentane	3.33	57	4765	9.53	ppb	90
41) Chloroform	5.28	83	23433	11.38	ppb	95
42) Bromochloromethane	5.13	49	5834	9.61	ppb	# 77
44) 1,1,1-TCA	5.49	97	10291	9.72	ppb	97
45) Cyclohexane	5.55	56	10690	7.86	ppb	92
46) 1,1-Dichloropropene	5.72	75	13939	9.38	ppb	88
47) 2,2,4-Trimethylpentane	6.13	57	23434	8.29	ppb	98
49) Carbon Tetrachloride	5.71	117	27595	11.13	ppb	98
50) Tert Amyl Methyl Ether	6.18	73	29219	10.51	ppb	91
51) Methylcyclopentane	4.67	56	1183	10.53	ppb	100
52) 1,2-DCA	6.01	62	17988	10.32	ppb	97
53) Benzene	5.97	78	37295	9.16	ppb	97
54) TCE	6.80	130	9688	10.21	ppb	89
55) 2-Pentanone	7.05	43	69658	109.93	ppb	98
56) 1,2-Dichloropropane	7.05	63	9121	9.93	ppb	# 96
57) Bromodichloromethane	7.40	83	18937	11.28	ppb	93
58) Methyl Cyclohexane	7.01	83	16172	8.59	ppb	97
59) Dibromomethane	7.18	174	18539	11.35	ppb	89
60) MIBK (methyl isobutyl ket	8.12	43	38238	46.36	ppb	93
61) 1-Bromo-2-chloroethane	7.73	63	5394	8.39	ppb	# 85
63) Cis-1,3-Dichloropropene	7.92	75	15986	9.34	ppb	# 85
64) Toluene	8.29	91	51983	9.70	ppb	96
65) Trans-1,3-Dichloropropene	8.56	75	16035	9.67	ppb	93
66) 1,1,2-TCA	8.75	97	11339	9.78	ppb	94
67) 2-Hexanone	9.05	43	26830	46.42	ppb	91
70) 1,2-EDB	9.29	107	13561	10.08	ppb	# 93
71) Tetrachloroethene	8.90	166	30260	10.40	ppb	98
72) 1-Chlorohexane	9.85	91	17406	9.06	ppb	100
73) 1,1,1,2-Tetrachloroethane	9.94	131	20390	10.88	ppb	97
74) m&p-Xylene	10.11	91	102955	19.66	ppb	98
75) o-Xylene	10.54	91	52039	9.44	ppb	95
76) Styrene	10.56	104	38808	9.54	ppb	99
78) 1,3-Dichloropropane	8.93	76	16074	9.30	ppb	92
79) Dibromochloromethane	9.17	129	19820	10.70	ppb	99
80) Chlorobenzene	9.84	112	45881	9.98	ppb	97
81) Ethylbenzene	9.98	91	65235	9.58	ppb	99
82) Bromoform	10.74	173	20602	11.49	ppb	92
84) Isopropylbenzene	10.95	105	71854	9.27	ppb	93
85) 1,1,2,2-Tetrachloroethane	11.27	83	12636	8.20	ppb	88
86) 1,2,3-Trichloropropane	11.31	110	6674	9.45	ppb	93
87) t-1,4-Dichloro-2-Butene	11.33	53	2984	8.43	ppb	90

(#) = qualifier out of range (m) = manual integration

Data File : M:\THOR\DATA\211111\1119T32.D  
 Acq On : 19 Nov 21 22:36  
 Sample : 211119B LCSD 10ug/L  
 Misc : IS&S 8/15/21

Vial: 32  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 22 11:04 2021

Quant Results File: T1109W.RES

Quant Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 10:21:13 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Compound	R.T.	QIon	Response	Conc	Unit	Qvalue
88) Bromobenzene	11.26	156	29098	10.22	ppb	91
89) n-Propylbenzene	11.40	91	76178	8.92	ppb	100
90) 4-Ethyltoluene	11.53	105	69513	8.78	ppb	91
91) 2-Chlorotoluene	11.48	91	52980	9.11	ppb	98
92) 1,3,5-Trimethylbenzene	11.60	105	65508	9.28	ppb	100
93) 4-Chlorotoluene	11.60	91	55295	9.38	ppb	95
94) Tert-Butylbenzene	11.95	119	73665	10.02	ppb	99
95) 1,2,4-Trimethylbenzene	12.00	105	63062	9.38	ppb	99
96) Sec-Butylbenzene	12.19	105	78238	9.21	ppb	92
97) p-Isopropyltoluene	12.35	119	79807	9.92	ppb	98
98) Benzyl Chloride	12.55	91	26413	8.75	ppb	97
99) 1,3-DCB	12.30	146	50837	9.78	ppb	93
100) 1,4-DCB	12.40	146	51599	9.61	ppb	96
101) n-Butylbenzene	12.80	91	52087	9.20	ppb	93
102) 1,2-DCB	12.80	146	47508	10.00	ppb	94
103) Hexachloroethane	13.09	201	21991	10.33	ppb	95
104) 1,2-Dibromo-3-chloropropan	13.65	157	5657	9.43	ppb	95
105) 1,2,4-Trichlorobenzene	14.57	180	37595	9.75	ppb	97
106) Hexachlorobutadiene	14.76	225	26942	10.69	ppb	96
107) Naphthalene	14.83	128	25544	8.18	ppb	99
108) 1,2,3-Trichlorobenzene	15.09	180	33771	10.09	ppb	91

# Quantitation Report


Data File : M:\THOR\DATA\211111\1119T32.D  
 Acq On : 19 Nov 21 22:36  
 Sample : 211119B LCSD 10ug/L  
 Misc : IS&S 8/15/21

Vial: 32  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 22 11:04 2021

Quant Results File: T1109W.RES

Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Wed Nov 10 10:21:13 2021  
 Response via : Initial Calibration




BFB

Data File : M:\THOR\DATA\211109\1109T13.D  
 Acq On : 9 Nov 21 11:23  
 Sample : 25ug/L BFB STD 10/29/21  
 Misc : IS&S 8/15/21

Vial: 1  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B




Spectrum Information: Average of 11.103 to 11.109 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	10936	PASS
75	95	30	60	50.2	34147	PASS
95	95	100	100	100.0	68029	PASS
96	95	5	9	6.4	4384	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	200	145.6	99061	PASS
175	174	5	9	8.1	8054	PASS
176	174	95	101	99.8	98904	PASS
177	176	5	9	6.1	6030	PASS

Data File : M:\MAX\DATA\211111\1111M21.D  
 Acq On : 11 Nov 21 18:10  
 Sample : 25ug/L BFB STD 10/29/21  
 Misc : IS&S 8/4/21

Vial: 1  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B



AutoFind: Scans 3041, 3042, 3043; Background Corrected with Scan 3027



Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.6	21067	PASS
75	95	30	60	56.9	58077	PASS
95	95	100	200	100.0	102045	PASS
96	95	5	9	6.4	6566	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	200	123.3	125821	PASS
175	174	5	9	8.8	11035	PASS
176	174	95	101	100.5	126427	PASS
177	176	5	9	7.0	8852	PASS

BFB

Data File : M:\MAX\DATA\211111\1115M01.D  
 Acq On : 15 Nov 21 8:32  
 Sample : 25ug/L BFB STD 10/29/21  
 Misc : IS&S 8/4/21

Vial: 1  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Method : M:\MAX\DATA\211111\M1111W.M (RTE Integrator)  
 Title : METHOD 8260B



AutoFind: Scans 3042, 3043, 3044; Background Corrected with Scan 3026

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	18637	PASS
75	95	30	60	59.5	58387	PASS
95	95	100	200	100.0	98139	PASS
96	95	5	9	6.7	6552	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	200	126.9	124581	PASS
175	174	5	9	7.8	9739	PASS
176	174	95	101	100.5	125251	PASS
177	176	5	9	6.9	8642	PASS





BFB

Data File : M:\THOR\DATA\211111\1119T30.D  
 Acq On : 19 Nov 21 21:46  
 Sample : 25ug/L BFB STD 10/29/21  
 Misc : IS&S 8/15/21

Vial: 30  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Method : M:\THOR\DATA\211109\T1109W.M (RTE Integrator)  
 Title : METHOD 8260B



Spectrum Information: Average of 11.103 to 11.109 min.

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	9028	PASS
75	95	30	60	52.5	29603	PASS
95	95	100	100	100.0	56432	PASS
96	95	5	9	6.7	3761	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	200	166.4	93899	PASS
175	174	5	9	7.7	7208	PASS
176	174	95	101	98.2	92219	PASS
177	176	5	9	6.5	5955	PASS

### THOR 8260 Standard Prep

THOR 8260 Water Calibration Curve										
0.3ug/L						Prepared By (Initials): CH				
Prepared: 11/9/2021										
Expires: 12/1/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Allquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 9	Various	0.3ug/L	5	Prepared 11/08/21	1/7/2022	N/A	3uL	50mL	P&T Water	0.3
VOA STD. 1	Absolute		50	Prepared 11/08/21	1/7/2022	N/A	5uL			5
VOA STD. 2	Phenova		100	Prepared 11/08/21	1/7/2022	N/A	2.5uL			5
VOA STD. TBA	Various		250	Prepared 11/08/21	12/1/2021	N/A	2uL			10
0.5ug/L										
Prepared: 11/9/2021										
Expires: 12/1/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Allquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 9	Various	0.5ug/L	5	Prepared 11/08/21	1/7/2022	N/A	5uL	50mL	P&T Water	0.5
VOA STD. 1	Absolute		50	Prepared 11/08/21	1/7/2022	N/A	10uL			10
VOA STD. 2	Phenova		100	Prepared 11/08/21	1/7/2022	N/A	5uL			10
VOA STD. TBA	Various		250	Prepared 11/08/21	12/1/2021	N/A	5uL			25
1.0ug/L										
Prepared: 11/9/2021										
Expires: 12/1/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Allquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 9	Various	1.0ug/L	5	Prepared 11/08/21	1/7/2022	N/A	10uL	50mL	P&T Water	1
VOA STD. 1	Absolute		50	Prepared 11/08/21	1/7/2022	N/A	20uL			20
VOA STD. 2	Phenova		100	Prepared 11/08/21	1/7/2022	N/A	10uL			20
VOA STD. TBA	Various		250	Prepared 11/08/21	12/1/2021	N/A	10uL			50
2.0ug/L										
Prepared: 11/9/2021										
Expires: 12/1/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Allquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 9	Various	2.0ug/L	5	Prepared 11/08/21	1/7/2022	N/A	20uL	50mL	P&T Water	2
VOA STD. 1	Absolute		50	Prepared 11/08/21	1/7/2022	N/A	30uL			30
VOA STD. 2	Phenova		100	Prepared 11/08/21	1/7/2022	N/A	15uL			30
VOA STD. TBA	Various		250	Prepared 11/08/21	12/1/2021	N/A	15uL			75
5ug/L										
Prepared: 11/9/2021										
Expires: 12/1/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Allquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	5ug/L	50	Prepared 11/08/21	1/7/2022	N/A	5uL	50mL	P&T Water	5
VOA STD. 8	Phenova		50	Prepared 11/08/21	12/1/2021	N/A	5uL			5
VOA STD. 1	Absolute		50	Prepared 11/08/21	1/7/2022	N/A	40uL			40
VOA STD. 2	Phenova		100	Prepared 11/08/21	1/7/2022	N/A	20uL			20
VOA STD. TBA	Various		250	Prepared 11/08/21	12/1/2021	N/A	20uL			100
10ug/L										
Prepared: 11/9/2021										
Expires: 12/1/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Allquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	10ug/L	50	Prepared 11/08/21	1/7/2022	N/A	10uL	50mL	P&T Water	10
VOA STD. 8	Phenova		50	Prepared 11/08/21	12/1/2021	N/A	10uL			10
VOA STD. 1	Absolute		50	Prepared 11/08/21	1/7/2022	N/A	50uL			50
VOA STD. 2	Phenova		100	Prepared 11/08/21	1/7/2022	N/A	25uL			50
VOA STD. TBA	Various		250	Prepared 11/08/21	12/1/2021	N/A	25uL			125

20ug/L											
Prepared: 11/9/2021											
Expires: 12/1/2021											
Initial Standard Information						Final Standard Information					
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)	
VOA STD. 7	Various	20ug/L	50	Prepared 11/08/21	1/7/2022	N/A	20uL	50mL	P&T Water	20	
VOA STD. 8	Phenova		50	Prepared 11/08/21	12/1/2021	N/A	20uL			20	
VOA STD. 1	Absolute		50	Prepared 11/08/21	1/7/2022	N/A	60uL			60	
VOA STD. 2	Phenova		100	Prepared 11/08/21	1/7/2022	N/A	30uL			60	
VOA STD. TBA	Various		250	Prepared 11/08/21	12/1/2021	N/A	30uL			150	
40ug/L											
Prepared: 11/9/2021											
Expires: 12/1/2021											
Initial Standard Information						Final Standard Information					
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)	
VOA STD. 7	Various	40ug/L	50	Prepared 11/08/21	1/7/2022	N/A	40uL	50mL	P&T Water	40	
VOA STD. 8	Phenova		50	Prepared 11/08/21	12/1/2021	N/A	40uL			40	
VOA STD. 1	Absolute		50	Prepared 11/08/21	1/7/2022	N/A	80uL			80	
VOA STD. 2	Phenova		100	Prepared 11/08/21	1/7/2022	N/A	40uL			80	
VOA STD. TBA	Various		250	Prepared 11/08/21	12/1/2021	N/A	35uL			175	
100ug/L											
Prepared: 11/9/2021											
Expires: 12/1/2021											
Initial Standard Information						Final Standard Information					
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)	
VOA STD. 7	Various	100ug/L	50	Prepared 11/08/21	1/7/2022	N/A	100uL	50mL	P&T Water	100	
VOA STD. 8	Phenova		50	Prepared 11/08/21	12/1/2021	N/A	100uL			100	
VOA STD. 1	Absolute		50	Prepared 11/08/21	1/7/2022	N/A	100uL			100	
VOA STD. 2	Phenova		100	Prepared 11/08/21	1/7/2022	N/A	50uL			100	
VOA STD. TBA	Various		250	Prepared 11/08/21	12/1/2021	N/A	40uL			200	
THOR 8260 Water Second Source (SS)											
Prepared: 11/9/2021						Prepared By (Initials): CH					
Expires: 12/1/2021											
Initial Standard Information						Final Standard Information					
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)	
VOA STD. 3	Phenova	8260 Water SS	100	Prepared 11/08/21	1/7/2022	N/A	25uL	50mL	P&T Water	50	
VOA STD. GASES	Phenova		50	Prepared 11/08/21	1/7/2022	N/A	10uL			10	
VOA STD. 0	Phenova		50	Prepared 11/08/21	1/7/2022	N/A	10uL			10	
VOA STD. 2-CEVE	Absolute		50	Prepared 11/08/21	11/8/2021	N/A	50uL			50	
VOA STD. 6	Various		50	Prepared 11/08/21	12/1/2021	N/A	10uL			10	
Voa STD. TBA	Various		8260 Water SS	250	Prepared 11/08/21	12/1/2021	N/A			25uL	250
8260 Water Continuing Calibrations (CCV)/ Lab Control Spikes (LCS)											
Prepared: 11/9/2021						Prepared By (Initials): CH					
Expires: 11/10/2021											
Initial Standard Information						Final Standard Information					
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)	
VOA STD. 7	Various	CCV/ LCS	50	Prepared 11/08/21	1/7/2022	N/A	10uL	50mL	P&T Water	10	
VOA STD. 8	Phenova		50	Prepared 11/08/21	12/1/2021	N/A	10uL			10	
VOA STD. 1	Absolute		50	Prepared 11/08/21	1/7/2022	N/A	50uL			50	
VOA STD. 2	Phenova		100	Prepared 11/08/21	1/7/2022	N/A	25uL			50	
VOA STD. TBA	Various		250	Prepared 11/08/21	12/1/2021	N/A	25uL			250	

## MAX 8260 Standard Prep

MAX 8260 Water Calibration Curve										
0.3ug/L						Prepared By (Initials): <u>CH</u>				
Prepared: 11/11/2021										
Expires: 12/1/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 9	Various	0.3ug/L	5	Prepared 11/08/21	1/7/2022	N/A	3uL	50mL	P&T Water	0.3
VOA STD. 1	Absolute		50	Prepared 11/08/21	1/7/2022	N/A	5uL			5
VOA STD. 2	Phenova		100	Prepared 11/08/21	1/7/2022	N/A	2.5uL			5
VOA STD. TBA	Various		250	Prepared 11/08/21	12/1/2021	N/A	2uL			10
0.5ug/L										
Prepared: 11/11/2021										
Expires: 12/1/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 9	Various	0.5ug/L	5	Prepared 11/08/21	1/7/2022	N/A	5uL	50mL	P&T Water	0.5
VOA STD. 1	Absolute		50	Prepared 11/08/21	1/7/2022	N/A	10uL			10
VOA STD. 2	Phenova		100	Prepared 11/08/21	1/7/2022	N/A	5uL			10
VOA STD. TBA	Various		250	Prepared 11/08/21	12/1/2021	N/A	5uL			25
1.0ug/L										
Prepared: 11/11/2021										
Expires: 12/1/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 9	Various	1.0ug/L	5	Prepared 11/08/21	1/7/2022	N/A	10uL	50mL	P&T Water	1
VOA STD. 1	Absolute		50	Prepared 11/08/21	1/7/2022	N/A	20uL			20
VOA STD. 2	Phenova		100	Prepared 11/08/21	1/7/2022	N/A	10uL			20
VOA STD. TBA	Various		250	Prepared 11/08/21	12/1/2021	N/A	10uL			50
2.0ug/L										
Prepared: 11/11/2021										
Expires: 12/1/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 9	Various	2.0ug/L	5	Prepared 11/08/21	1/7/2022	N/A	20uL	50mL	P&T Water	2
VOA STD. 1	Absolute		50	Prepared 11/08/21	1/7/2022	N/A	30uL			30
VOA STD. 2	Phenova		100	Prepared 11/08/21	1/7/2022	N/A	15uL			30
VOA STD. TBA	Various		250	Prepared 11/08/21	12/1/2021	N/A	15uL			75
5ug/L										
Prepared: 11/11/2021										
Expires: 12/1/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	5ug/L	50	Prepared 11/08/21	1/7/2022	N/A	5uL	50mL	P&T Water	5
VOA STD. 8	Phenova		50	Prepared 11/08/21	12/1/2021	N/A	5uL			5
VOA STD. 1	Absolute		50	Prepared 11/08/21	1/7/2022	N/A	40uL			40
VOA STD. 2	Phenova		100	Prepared 11/08/21	1/7/2022	N/A	20uL			20
VOA STD. TBA	Various		250	Prepared 11/08/21	12/1/2021	N/A	20uL			100
10ug/L										
Prepared: 11/11/2021										
Expires: 12/1/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	10ug/L	50	Prepared 11/08/21	1/7/2022	N/A	10uL	50mL	P&T Water	10
VOA STD. 8	Phenova		50	Prepared 11/08/21	12/1/2021	N/A	10uL			10
VOA STD. 1	Absolute		50	Prepared 11/08/21	1/7/2022	N/A	50uL			50
VOA STD. 2	Phenova		100	Prepared 11/08/21	1/7/2022	N/A	25uL			50
VOA STD. TBA	Various		250	Prepared 11/08/21	12/1/2021	N/A	25uL			125

20ug/L										
Prepared: 11/11/2021										
Expires: 12/1/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	20ug/L	50	Prepared 11/08/21	1/7/2022	N/A	20uL	50mL	P&T Water	20
VOA STD. 8	Phenova		50	Prepared 11/08/21	12/1/2021	N/A	20uL			20
VOA STD. 1	Absolute		50	Prepared 11/08/21	1/7/2022	N/A	60uL			60
VOA STD. 2	Phenova		100	Prepared 11/08/21	1/7/2022	N/A	30uL			60
VOA STD. TBA	Various		250	Prepared 11/08/21	12/1/2021	N/A	30uL			150
40ug/L										
Prepared: 11/11/2021										
Expires: 12/1/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	40ug/L	50	Prepared 11/08/21	1/7/2022	N/A	40uL	50mL	P&T Water	40
VOA STD. 8	Phenova		50	Prepared 11/08/21	12/1/2021	N/A	40uL			40
VOA STD. 1	Absolute		50	Prepared 11/08/21	1/7/2022	N/A	80uL			80
VOA STD. 2	Phenova		100	Prepared 11/08/21	1/7/2022	N/A	40uL			80
VOA STD. TBA	Various		250	Prepared 11/08/21	12/1/2021	N/A	35uL			175
100ug/L										
Prepared: 11/11/2021										
Expires: 12/1/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	100ug/L	50	Prepared 11/08/21	1/7/2022	N/A	100uL	50mL	P&T Water	100
VOA STD. 8	Phenova		50	Prepared 11/08/21	12/1/2021	N/A	100uL			100
VOA STD. 1	Absolute		50	Prepared 11/08/21	1/7/2022	N/A	100uL			100
VOA STD. 2	Phenova		100	Prepared 11/08/21	1/7/2022	N/A	50uL			100
VOA STD. TBA	Various		250	Prepared 11/08/21	12/1/2021	N/A	40uL			200
MAX 8260 Water Second Source (SS)										
Prepared: 11/11/2021										
Expires: 12/1/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 3	Phenova	8260 Water SS	100	Prepared 11/08/21	1/7/2022	N/A	25uL	50mL	P&T Water	50
VOA STD. GASES	Phenova		50	Prepared 11/08/21	1/7/2022	N/A	10uL			10
VOA STD. 0	Phenova		50	Prepared 11/08/21	1/7/2022	N/A	10uL			10
VOA STD. 2-CEVE	Absolute		50	Prepared 11/08/21	11/8/2021	N/A	50uL			50
VOA STD. 6	Various		50	Prepared 11/08/21	12/1/2021	N/A	10uL			10
VOA STD. TBA	Various		250	Prepared 11/08/21	12/1/2021	N/A	25uL			250
8260 Water Continuing Calibrations (CCV)/ Lab Control Spikes (LCS)										
Prepared: 11/11/2021										
Expires: 11/12/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	CCV/ LCS	50	Prepared 11/08/21	1/7/2022	N/A	10uL	50mL	P&T Water	10
VOA STD. 8	Phenova		50	Prepared 11/08/21	12/1/2021	N/A	10uL			10
VOA STD. 1	Absolute		50	Prepared 11/08/21	1/7/2022	N/A	50uL			50
VOA STD. 2	Phenova		100	Prepared 11/08/21	1/7/2022	N/A	25uL			50
VOA STD. TBA	Various		250	Prepared 11/08/21	12/1/2021	N/A	25uL			250

## Injection Log

Directory: M:\THOR\DATA\211109\

Line	Vial	FileName	Multiplier	SampleName	Misc Info	Injected
1	1	1109T13.D	1	25ug/L BFB STD 10/29/21	IS&S 8/15/21	9 Nov 21 11:23
2	2	1109T14.D	1	0.3ug/L VOC STD 11/9/21	IS&S 8/15/21	9 Nov 21 11:48
3	3	1109T15.D	1	0.5ug/L VOC STD 11/9/21	IS&S 8/15/21	9 Nov 21 12:13
4	4	1109T16.D	1	1ug/L VOC STD 11/9/21	IS&S 8/15/21	9 Nov 21 12:38
5	5	1109T17.D	1	2ug/L VOC STD 11/9/21	IS&S 8/15/21	9 Nov 21 13:03
6	6	1109T18.D	1	5ug/L VOC STD 11/9/21	IS&S 8/15/21	9 Nov 21 13:28
7	7	1109T19.D	1	10ug/L VOC STD 11/9/21	IS&S 8/15/21	9 Nov 21 13:52
8	8	1109T20.D	1	20ug/L VOC STD 11/9/21	IS&S 8/15/21	9 Nov 21 14:17
9	9	1109T21.D	1	40ug/L VOC STD 11/9/21	IS&S 8/15/21	9 Nov 21 14:42
10	10	1109T22.D	1	100ug/L VOC STD 11/9/21	IS&S 8/15/21	9 Nov 21 15:07
11	12	1109T24.D	1	(SS) 10ug/L VOC STD 11/9/21	IS&S 8/15/21	9 Nov 21 15:57

## Injection Log

Directory: M:\MAX\DATA\211111\

Line	Vial	FileName	Multiplier	SampleName	Misc Info	Injected
1	1	1111M21.D	1	25ug/L BFB STD 10/29/21	IS&S 8/4/21	11 Nov 21 18:10
2	2	1111M22.D	1	0.3ug/L VOC STD 11/11/21	IS&S 8/4/21	11 Nov 21 18:38
3	3	1111M23.D	1	0.5ug/L VOC STD 11/11/21	IS&S 8/4/21	11 Nov 21 19:07
4	4	1111M24.D	1	1ug/L VOC STD 11/11/21	IS&S 8/4/21	11 Nov 21 19:35
5	5	1111M25.D	1	2ug/L VOC STD 11/11/21	IS&S 8/4/21	11 Nov 21 20:03
6	6	1111M26.D	1	5ug/L VOC STD 11/11/21	IS&S 8/4/21	11 Nov 21 20:32
7	7	1111M27.D	1	10ug/L VOC STD 11/11/21	IS&S 8/4/21	11 Nov 21 21:00
8	8	1111M28.D	1	20ug/L VOC STD 11/11/21	IS&S 8/4/21	11 Nov 21 21:28
9	9	1111M29.D	1	40ug/L VOC STD 11/11/21	IS&S 8/4/21	11 Nov 21 21:57
10	10	1111M30.D	1	100ug/L VOC STD 11/11/21	IS&S 8/4/21	11 Nov 21 22:25
11	12	1111M32.D	1	(SS) 10ug/L VOC STD 11/11/21	IS&S 8/4/21	11 Nov 21 23:22

# Injection Log

Directory: M:\MAX\DATA\211111\

Line	Vial	FileName	Multiplier	SampleName	Misc Info	Injected
1	1	1115M01.D	1	25ug/L BFB STD 10/29/21	IS&S 8/4/21	15 Nov 21 8:32
2	3	1115M03.D	1	211115A CCV/LCS 10ug/L	IS&S 8/4/21	15 Nov 21 9:28
3	4	1115M04.D	1	211115A LCSD 10ug/L	IS&S 8/4/21	15 Nov 21 9:57
4	8	1115M08.D	1	211115A BLK	IS&S 8/4/21	15 Nov 21 11:50
5	12	1115M12.D	1	BA46114W01	IS&S 8/4/21	15 Nov 21 13:44
6	13	1115M13.D	1	BA46115W01	IS&S 8/4/21	15 Nov 21 14:12
7	14	1115M14.D	1	BA46116W01	IS&S 8/4/21	15 Nov 21 14:40
8	25	1115M25.D	1	Ending CCV 10ug/L 11/15/21	IS&S 8/4/21	15 Nov 21 19:52



# Injection Log

Directory: M:\THOR\DATA\211111\

Line	Vial	FileName	Multiplier	SampleName	Misc Info	Injected
1	30	1119T30.D	1	25ug/L BFB STD 10/29/21	IS&S 8/15/21	19 Nov 21 21:46
2	31	1119T31.D	1	211119B CCV/LCS 10ug/L	IS&S 8/15/21	19 Nov 21 22:11
3	32	1119T32.D	1	211119B LCSD 10ug/L	IS&S 8/15/21	19 Nov 21 22:36
4	37	1119T37.D	1	211119B BLK	IS&S 8/15/21	20 Nov 21 00:39
5	38	1119T38.D	1	BA46117W07	IS&S 8/15/21	20 Nov 21 1:03
6	52	1119T52.D	1	Ending CCV 10ug/L 11/19/21	IS&S 8/15/21	20 Nov 21 6:47

**ORGANICS**  
**Calibration Data**

VOLATILE ORGANIC ANALYSIS BY  
EPA METHOD 8260B

Form 6  
Initial Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: \_\_\_\_\_

SDG No: \_\_\_\_\_  
Initial Cal. Date: 8/25/2021  
Instrument: Max

Initials: \_\_\_\_\_

0825M12.D    0825M13.D    0825M14.D    0825M15.D    0825M16.D    0825M17.D    0825M18.D    0825M19.D    0825M20.D

	Compound	1	2	3	4	5	6	7	8	9		Avg	%RSD	Type	r <sup>2</sup>	Q	MRF
1	I Fluorobenzene (IS)																
2	S Dibromofluoromethane(S)	0.3523	0.3417	0.2807	0.2859	0.2870	0.2956	0.2984	0.3009	0.2709		0.30	9.1	S			
3	S 1,2-DCA-D4(S)	0.2194	0.2154	0.1883	0.1930	0.1953	0.1908	0.1985	0.2034	0.1791		0.20	6.5	S			
4	I Chlorobenzene-D5 (IS)																
5	S Toluene-D8(S)	1.390	1.326	1.153	1.099	1.153	1.163	1.121	1.122	1.024		1.2	9.8	S			
6	S 4-Bromofluorobenzene(S)	0.5362	0.5171	0.4075	0.4294	0.4615	0.4643	0.4388	0.4514	0.4103		0.46	9.7	S			
7	I 1,4-Dichlorobenzene-D (IS)																
8																	
9																	
10																	
11																	
12																	
13																	
14																	
15																	
16																	
17																	
18																	
19																	
20																	
21																	
22																	
23																	
24																	
25																	
26																	
27																	
28																	
29																	
30																	
31																	
32																	
33																	
34																	
35																	

Quantitation Report (Not Reviewed)

Data File : M:\MAX\DATA\210825\0825M12.D  
 Acq On : 25 Aug 21 15:15  
 Sample : 0.3ug/L VOC STD 8/25/21  
 Misc : IS&S 6/4/21

Vial: 2  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Aug 26 16:25 2021

Quant Results File: M0825SUR.RES

Quant Method : M:\MAX\DATA\210825\M0825SUR.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Thu Aug 26 11:16:48 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260\_081021

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.21	96	268418	25.00	ppb	0.00
4) Chlorobenzene-D5 (IS)	9.41	117	221472	25.00	ppb	0.00
7) 1,4-Dichlorobenzene-D (IS)	11.75	152	137587	25.00	ppb	0.00
<b>System Monitoring Compounds</b>						
2) Dibromofluoromethane(S)	5.41	111	18913	5.84	ppb	0.00
Spiked Amount 25.000			Recovery =	23.372%		
3) 1,2-DCA-D4(S)	5.81	65	11779	5.54	ppb	0.00
Spiked Amount 25.000			Recovery =	22.148%		
5) Toluene-D8(S)	7.95	98	61590	5.93	ppb	0.00
Spiked Amount 25.000			Recovery =	23.720%		
6) 4-Bromofluorobenzene(S)	10.60	95	23749	5.86	ppb	0.00
Spiked Amount 25.000			Recovery =	23.444%		

Target Compounds Qvalue

Quantitation Report


Data File : M:\MAX\DATA\210825\0825M12.D  
Acq On : 25 Aug 21 15:15  
Sample : 0.3ug/L VOC STD 8/25/21  
Misc : IS&S 6/4/21

Vial: 2  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Aug 26 16:25 2021

Quant Results File: M0825SUR.RES

Method : M:\MAX\DATA\210825\M0825SUR.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Aug 26 11:16:48 2021  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data File : M:\MAX\DATA\210825\0825M13.D  
 Acq On : 25 Aug 21 15:43  
 Sample : 0.5ug/L VOC STD 8/25/21  
 Misc : IS&S 6/4/21

Vial: 3  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Aug 26 16:25 2021

Quant Results File: M0825SUR.RES

Quant Method : M:\MAX\DATA\210825\M0825SUR.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Thu Aug 26 11:16:48 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260\_081021

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.21	96	270425	25.00	ppb	0.00
4) Chlorobenzene-D5 (IS)	9.41	117	226950	25.00	ppb	0.00
7) 1,4-Dichlorobenzene-D (IS)	11.75	152	138629	25.00	ppb	0.00
<b>System Monitoring Compounds</b>						
2) Dibromofluoromethane(S)	5.42	111	18480	5.67	ppb	0.00
Spiked Amount				25.000		
					Recovery =	22.664%
3) 1,2-DCA-D4(S)	5.81	65	11650	5.44	ppb	0.00
Spiked Amount				25.000		
					Recovery =	21.744%
5) Toluene-D8(S)	7.95	98	60175	5.65	ppb	0.00
Spiked Amount				25.000		
					Recovery =	22.616%
6) 4-Bromofluorobenzene(S)	10.60	95	23472	5.65	ppb	0.00
Spiked Amount				25.000		
					Recovery =	22.612%

Target Compounds

Qvalue

Quantitation Report


Data File : M:\MAX\DATA\210825\0825M13.D  
Acq On : 25 Aug 21 15:43  
Sample : 0.5ug/L VOC STD 8/25/21  
Misc : IS&S 6/4/21

Vial: 3  
Operator: LP, DG, CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Aug 26 16:25 2021

Quant Results File: M0825SUR.RES

Method : M:\MAX\DATA\210825\M0825SUR.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Aug 26 11:16:48 2021  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data File : M:\MAX\DATA\210825\0825M14.D  
 Acq On : 25 Aug 21 16:11  
 Sample : 1ug/L VOC STD 8/25/21  
 Misc : IS&S 6/4/21

Vial: 4  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Aug 26 16:25 2021

Quant Results File: M0825SUR.RES

Quant Method : M:\MAX\DATA\210825\M0825SUR.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Thu Aug 26 11:16:48 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260\_081021

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.22	96	261019	25.00	ppb	0.00
4) Chlorobenzene-D5 (IS)	9.41	117	222702	25.00	ppb	0.00
7) 1,4-Dichlorobenzene-D (IS)	11.75	152	137225	25.00	ppb	0.00
<b>System Monitoring Compounds</b>						
2) Dibromofluoromethane(S)	5.41	111	29305	9.31	ppb	0.00
Spiked Amount						
						Recovery = 37.236%
3) 1,2-DCA-D4(S)	5.81	65	19664	9.51	ppb	0.00
Spiked Amount						
						Recovery = 38.024%
5) Toluene-D8(S)	7.95	98	102711	9.84	ppb	0.00
Spiked Amount						
						Recovery = 39.340%
6) 4-Bromofluorobenzene(S)	10.60	95	36297	8.91	ppb	0.00
Spiked Amount						
						Recovery = 35.632%

Target Compounds

Qvalue



Quantitation Report


Data File : M:\MAX\DATA\210825\0825M14.D  
Acq On : 25 Aug 21 16:11  
Sample : 1ug/L VOC STD 8/25/21  
Misc : IS&S 6/4/21

Vial: 4  
Operator: LP, DG, CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Aug 26 16:25 2021

Quant Results File: M0825SUR.RES

Method : M:\MAX\DATA\210825\M0825SUR.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Aug 26 11:16:48 2021  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data File : M:\MAX\DATA\210825\0825M15.D  
 Acq On : 25 Aug 21 16:39  
 Sample : 2ug/L VOC STD 8/25/21  
 Misc : IS&S 6/4/21

Vial: 5  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Aug 26 16:25 2021

Quant Results File: M0825SUR.RES

Quant Method : M:\MAX\DATA\210825\M0825SUR.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Thu Aug 26 11:16:48 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260\_081021

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.21	96	260699	25.00	ppb	0.00
4) Chlorobenzene-D5 (IS)	9.42	117	218570	25.00	ppb	0.00
7) 1,4-Dichlorobenzene-D (IS)	11.75	152	137104	25.00	ppb	0.00
<b>System Monitoring Compounds</b>						
2) Dibromofluoromethane(S)	5.41	111	29818	9.48	ppb	0.00
Spiked Amount	25.000		Recovery	=	37.936%	
3) 1,2-DCA-D4(S)	5.82	65	20128	9.74	ppb	0.00
Spiked Amount	25.000		Recovery	=	38.968%	
5) Toluene-D8(S)	7.95	98	96059	9.37	ppb	0.00
Spiked Amount	25.000		Recovery	=	37.488%	
6) 4-Bromofluorobenzene(S)	10.60	95	37545	9.39	ppb	0.00
Spiked Amount	25.000		Recovery	=	37.556%	

Target Compounds

Qvalue

Quantitation Report


Data File : M:\MAX\DATA\210825\0825M15.D  
Acq On : 25 Aug 21 16:39  
Sample : 2ug/L VOC STD 8/25/21  
Misc : IS&S 6/4/21

Vial: 5  
Operator: LP, DG, CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Aug 26 16:25 2021

Quant Results File: M0825SUR.RES

Method : M:\MAX\DATA\210825\M0825SUR.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Aug 26 11:16:48 2021  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data File : M:\MAX\DATA\210825\0825M16.D  
 Acq On : 25 Aug 21 17:07  
 Sample : 5ug/L VOC STD 8/25/21  
 Misc : IS&S 6/4/21

Vial: 6  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Aug 26 16:25 2021

Quant Results File: M0825SUR.RES

Quant Method : M:\MAX\DATA\210825\M0825SUR.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Thu Aug 26 11:16:48 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260\_081021

Internal Standards	R.T.	Q Ion	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.21	96	261599	25.00	ppb	0.00
4) Chlorobenzene-D5 (IS)	9.41	117	219379	25.00	ppb	0.00
7) 1,4-Dichlorobenzene-D (IS)	11.75	152	136215	25.00	ppb	0.00
System Monitoring Compounds						
2) Dibromofluoromethane(S)	5.41	111	75090	23.80	ppb	0.00
Spiked Amount	25.000					
					Recovery =	95.204%
3) 1,2-DCA-D4(S)	5.81	65	51096	24.65	ppb	0.00
Spiked Amount	25.000				Recovery =	98.580%
5) Toluene-D8(S)	7.95	98	252960	24.59	ppb	0.00
Spiked Amount	25.000				Recovery =	98.356%
6) 4-Bromofluorobenzene(S)	10.60	95	101253	25.23	ppb	0.00
Spiked Amount	25.000				Recovery =	100.908%

Target Compounds

Qvalue

Quantitation Report


Data File : M:\MAX\DATA\210825\0825M16.D  
Acq On : 25 Aug 21 17:07  
Sample : 5ug/L VOC STD 8/25/21  
Misc : IS&S 6/4/21

Vial: 6  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Aug 26 16:25 2021

Quant Results File: M0825SUR.RES

Method : M:\MAX\DATA\210825\M0825SUR.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Aug 26 11:16:48 2021  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data File : M:\MAX\DATA\210825\0825M17.D  
 Acq On : 25 Aug 21 17:35  
 Sample : 10ug/L VOC STD 8/25/21  
 Misc : IS&S 6/4/21

Vial: 7  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Aug 26 16:25 2021

Quant Results File: M0825SUR.RES

Quant Method : M:\MAX\DATA\210825\M0825SUR.M (RTE Integrator)

Title : METHOD 8260B  
 Last Update : Thu Aug 26 11:16:48 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260\_081021

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.21	96	260876	25.00	ppb	0.00
4) Chlorobenzene-D5 (IS)	9.41	117	215380	25.00	ppb	0.00
7) 1,4-Dichlorobenzene-D (IS)	11.75	152	136295	25.00	ppb	0.00
System Monitoring Compounds						
2) Dibromofluoromethane(S)	5.42	111	77116	24.51	ppb	0.00
Spiked Amount	25.000		Recovery	=	98.044%	
3) 1,2-DCA-D4(S)	5.82	65	49768	24.07	ppb	0.00
Spiked Amount	25.000		Recovery	=	96.284%	
5) Toluene-D8(S)	7.95	98	250522	24.80	ppb	0.00
Spiked Amount	25.000		Recovery	=	99.216%	
6) 4-Bromofluorobenzene(S)	10.60	95	100010	25.38	ppb	0.00
Spiked Amount	25.000		Recovery	=	101.520%	

Target Compounds

Qvalue

Quantitation Report


Data File : M:\MAX\DATA\210825\0825M17.D  
Acq On : 25 Aug 21 17:35  
Sample : 10ug/L VOC STD 8/25/21  
Misc : IS&S 6/4/21

Vial: 7  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Aug 26 16:25 2021

Quant Results File: M0825SUR.RES

Method : M:\MAX\DATA\210825\M0825SUR.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Aug 26 11:16:48 2021  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data File : M:\MAX\DATA\210825\0825M18.D  
 Acq On : 25 Aug 21 18:03  
 Sample : 20ug/L VOC STD 8/25/21  
 Misc : IS&S 6/4/21

Vial: 8  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Aug 26 16:25 2021

Quant Results File: M0825SUR.RES

Quant Method : M:\MAX\DATA\210825\M0825SUR.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Thu Aug 26 11:16:48 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260\_081021

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.21	96	258006	25.00	ppb	0.00
4) Chlorobenzene-D5 (IS)	9.41	117	222674	25.00	ppb	0.00
7) 1,4-Dichlorobenzene-D (IS)	11.75	152	141752	25.00	ppb	0.00
<b>System Monitoring Compounds</b>						
2) Dibromofluoromethane(S)	5.42	111	153975	49.49	ppb	0.00
Spiked Amount						Recovery = 197.940%
3) 1,2-DCA-D4(S)	5.81	65	102408	50.08	ppb	0.00
Spiked Amount						Recovery = 200.332%
5) Toluene-D8(S)	7.95	98	499120	47.80	ppb	0.00
Spiked Amount						Recovery = 191.196%
6) 4-Bromofluorobenzene(S)	10.60	95	195414	47.97	ppb	0.00
Spiked Amount						Recovery = 191.868%

Target Compounds

Qvalue



Quantitation Report


Data File : M:\MAX\DATA\210825\0825M18.D  
Acq On : 25 Aug 21 18:03  
Sample : 20ug/L VOC STD 8/25/21  
Misc : IS&S 6/4/21

Vial: 8  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Aug 26 16:25 2021

Quant Results File: M0825SUR.RES

Method : M:\MAX\DATA\210825\M0825SUR.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Aug 26 11:16:48 2021  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data File : M:\MAX\DATA\210825\0825M19.D  
 Acq On : 25 Aug 21 18:31  
 Sample : 40ug/L VOC STD 8/25/21  
 Misc : IS&S 6/4/21

Vial: 9  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Aug 26 16:25 2021

Quant Results File: M0825SUR.RES

Quant Method : M:\MAX\DATA\210825\M0825SUR.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Thu Aug 26 11:16:48 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260\_081021

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.21	96	251853	25.00	ppb	0.00
4) Chlorobenzene-D5 (IS)	9.41	117	216925	25.00	ppb	0.00
7) 1,4-Dichlorobenzene-D (IS)	11.75	152	140689	25.00	ppb	0.00
<b>System Monitoring Compounds</b>						
2) Dibromofluoromethane(S)	5.41	111	151584	49.91	ppb	0.00
Spiked Amount				25.000		
					Recovery = 199.628%	
3) 1,2-DCA-D4(S)	5.81	65	102456	51.33	ppb	0.00
Spiked Amount				25.000		
					Recovery = 205.320%	
5) Toluene-D8(S)	7.95	98	486936	47.87	ppb	0.00
Spiked Amount				25.000		
					Recovery = 191.472%	
6) 4-Bromofluorobenzene(S)	10.60	95	195822	49.34	ppb	0.00
Spiked Amount				25.000		
					Recovery = 197.364%	

Target Compounds

Qvalue

Quantitation Report


Data File : M:\MAX\DATA\210825\0825M19.D  
Acq On : 25 Aug 21 18:31  
Sample : 40ug/L VOC STD 8/25/21  
Misc : IS&S 6/4/21

Vial: 9  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Aug 26 16:25 2021

Quant Results File: M0825SUR.RES

Method : M:\MAX\DATA\210825\M0825SUR.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Aug 26 11:16:48 2021  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data File : M:\MAX\DATA\210825\0825M20.D  
 Acq On : 25 Aug 21 18:59  
 Sample : 100ug/L VOC STD 8/25/21  
 Misc : IS&S 6/4/21

Vial: 10  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Aug 26 16:25 2021

Quant Results File: M0825SUR.RES

Quant Method : M:\MAX\DATA\210825\M0825SUR.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Thu Aug 26 11:16:48 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260\_081021

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.21	96	251268	25.00	ppb	0.00
4) Chlorobenzene-D5 (IS)	9.41	117	218191	25.00	ppb	0.00
7) 1,4-Dichlorobenzene-D (IS)	11.75	152	142788	25.00	ppb	0.00
<b>System Monitoring Compounds</b>						
2) Dibromofluoromethane(S)	5.42	111	272268	89.85	ppb	0.00
Spiked Amount 25.000			Recovery =	359.396%		
3) 1,2-DCA-D4 (S)	5.81	65	179968	90.37	ppb	0.00
Spiked Amount 25.000			Recovery =	361.496%		
5) Toluene-D8 (S)	7.95	98	893556	87.33	ppb	0.00
Spiked Amount 25.000			Recovery =	349.324%		
6) 4-Bromofluorobenzene(S)	10.60	95	358053	89.70	ppb	0.00
Spiked Amount 25.000			Recovery =	358.780%		

Target Compounds

Qvalue

Quantitation Report


Data File : M:\MAX\DATA\210825\0825M20.D  
Acq On : 25 Aug 21 18:59  
Sample : 100ug/L VOC STD 8/25/21  
Misc : IS&S 6/4/21

Vial: 10  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Aug 26 16:25 2021

Quant Results File: M0825SUR.RES

Method : M:\MAX\DATA\210825\M0825SUR.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Aug 26 11:16:48 2021  
Response via : Initial Calibration



VOLATILE ORGANIC ANALYSIS  
VOLATILE ORGANIC COMPOUNDS

Form 6  
Initial Calibration

Lab Name: APPL, Inc.

SDG No: \_\_\_\_\_

Case No: \_\_\_\_\_

Initial Cal. Date: 8/25/2021

Matrix: \_\_\_\_\_

Instrument: Max

Initials: \_\_\_\_\_

0825M23.D    0825M24.D    0825M25.D    0825M26.D    0825M27.D    0825M28.D    0825M29.D

	Compound	1	2	3	4	5	6	7				Avg	%RSD	Type	r <sup>2</sup>	Q	MRF
1	I Fluorobenzene (IS)																
2	TMHBI Gasoline C6-C10	13.8	5.689	3.019	1.290	0.8206	0.7117	0.6349				3.7	130	TMHB	0.999		
3	TMHB Chlorobenzene-D5 (IS)																
4	TMHB 1,4-Dichlorobenzene (IS)																
5																	
6																	
7																	
8																	
9																	
10																	
11																	
12																	
13																	
14																	
15																	
16																	
17																	
18																	
19																	
20																	
21																	
22																	
23																	
24																	
25																	
26																	
27																	
28																	
29																	
30																	
31																	
32																	
33																	
34																	
35																	

Quantitation Report (QT Reviewed)

Data File : M:\MAX\DATA\210825\0825M23.D  
 Acq On : 25 Aug 21 20:23  
 Sample : 20ug/L GAS STD 8/25/21  
 Misc : IS&S 6/4/21

Vial: 13  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Aug 26 16:15 2021

Quant Results File: MGAS0825.RES

Quant Method : M:\MAX\DATA\210825\MGAS0825.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Thu Aug 26 16:13:10 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260\_081021

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.21	TIC	284811	25.00	ppb	0.00
3) Chlorobenzene-D5 (IS)	11.75	TIC	236410m	25.00	ppb	0.00
4) 1,4-Dichlorobenzene (IS)	10.94	TIC	14670m	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Gasoline C6-C10	7.95	TIC	3136582m	38.03	ppb	100

Quantitation Report


Data File : M:\MAX\DATA\210825\0825M23.D  
Acq On : 25 Aug 21 20:23  
Sample : 20ug/L GAS STD 8/25/21  
Misc : IS&S 6/4/21

Vial: 13  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Aug 26 16:15 2021

Quant Results File: MGAS0825.RES

Method : M:\MAX\DATA\210825\MGAS0825.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Aug 26 16:19:36 2021  
Response via : Initial Calibration





Quantitation Report (QT Reviewed)

Data File : M:\MAX\DATA\210825\0825M24.D  
 Acq On : 25 Aug 21 20:51  
 Sample : 50ug/L GAS STD 8/25/21  
 Misc : IS&S 6/4/21

Vial: 14  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Aug 26 16:15 2021

Quant Results File: MGAS0825.RES

Quant Method : M:\MAX\DATA\210825\MGAS0825.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Thu Aug 26 16:13:10 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260\_081021

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.21	TIC	285081	25.00	ppb	0.00
3) Chlorobenzene-D5 (IS)	11.75	TIC	248593m	25.00	ppb	0.00
4) 1,4-Dichlorobenzene (IS)	10.94	TIC	21251m	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Gasoline C6-C10	7.95	TIC	3243874m	61.97	ppb	100

Quantitation Report


Data File : M:\MAX\DATA\210825\0825M24.D  
Acq On : 25 Aug 21 20:51  
Sample : 50ug/L GAS STD 8/25/21  
Misc : IS&S 6/4/21

Vial: 14  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Aug 26 16:15 2021

Quant Results File: MGAS0825.RES

Method : M:\MAX\DATA\210825\MGAS0825.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Aug 26 16:19:36 2021  
Response via : Initial Calibration



Quantitation Report (QT Reviewed)

Data File : M:\MAX\DATA\210825\0825M25.D  
 Acq On : 25 Aug 21 21:19  
 Sample : 100ug/L GAS STD 8/25/21  
 Misc : IS&S 6/4/21

Vial: 15  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Aug 26 16:16 2021

Quant Results File: MGAS0825.RES

Quant Method : M:\MAX\DATA\210825\MGAS0825.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Thu Aug 26 16:13:10 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260\_081021

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.21	TIC	286586	25.00	ppb	0.00
3) Chlorobenzene-D5 (IS)	11.75	TIC	245880m	25.00	ppb	0.00
4) 1,4-Dichlorobenzene (IS)	10.94	TIC	32801m	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Gasoline C6-C10	7.95	TIC	3460677m	107.56	ppb	100

Quantitation Report


Data File : M:\MAX\DATA\210825\0825M25.D  
Acq On : 25 Aug 21 21:19  
Sample : 100ug/L GAS STD 8/25/21  
Misc : IS&S 6/4/21

Vial: 15  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Aug 26 16:16 2021

Quant Results File: MGAS0825.RES

Method : M:\MAX\DATA\210825\MGAS0825.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Aug 26 16:19:36 2021  
Response via : Initial Calibration



Quantitation Report (QT Reviewed)

Data File : M:\MAX\DATA\210825\0825M26.D  
 Acq On : 25 Aug 21 21:47  
 Sample : 300ug/L GAS STD 8/25/21  
 Misc : IS&S 6/4/21

Vial: 16  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Aug 26 16:16 2021

Quant Results File: MGAS0825.RES

Quant Method : M:\MAX\DATA\210825\MGAS0825.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Thu Aug 26 16:13:10 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260\_081021

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.21	TIC	280163	25.00	ppb	0.00
3) Chlorobenzene-D5 (IS)	11.75	TIC	264646m	25.00	ppb	0.00
4) 1,4-Dichlorobenzene (IS)	10.94	TIC	87973m	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Gasoline C6-C10	7.95	TIC	4335414m	329.97	ppb	100

Quantitation Report


Data File : M:\MAX\DATA\210825\0825M26.D  
Acq On : 25 Aug 21 21:47  
Sample : 300ug/L GAS STD 8/25/21  
Misc : IS&S 6/4/21

Vial: 16  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Aug 26 16:16 2021

Quant Results File: MGAS0825.RES

Method : M:\MAX\DATA\210825\MGAS0825.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Aug 26 16:19:36 2021  
Response via : Initial Calibration



Quantitation Report (QT Reviewed)

Data File : M:\MAX\DATA\210825\0825M27.D  
 Acq On : 25 Aug 21 22:14  
 Sample : 600ug/L GAS STD 8/25/21  
 Misc : IS&S 6/4/21

Vial: 17  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Aug 26 16:18 2021

Quant Results File: MGAS0825.RES

Quant Method : M:\MAX\DATA\210825\MGAS0825.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Thu Aug 26 16:13:10 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260\_081021

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.21	TIC	283991	25.00	ppb	0.00
3) Chlorobenzene-D5 (IS)	11.75	TIC	290103m	25.00	ppb	0.00
4) 1,4-Dichlorobenzene (IS)	10.94	TIC	180429m	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Gasoline C6-C10	7.95	TIC	5593097m	606.10	ppb	100

Quantitation Report


Data File : M:\MAX\DATA\210825\0825M27.D  
Acq On : 25 Aug 21 22:14  
Sample : 600ug/L GAS STD 8/25/21  
Misc : IS&S 6/4/21

Vial: 17  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Aug 26 16:18 2021

Quant Results File: MGAS0825.RES

Method : M:\MAX\DATA\210825\MGAS0825.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Aug 26 16:19:36 2021  
Response via : Initial Calibration





Quantitation Report (QT Reviewed)

Data File : M:\MAX\DATA\210825\0825M28.D  
 Acq On : 25 Aug 21 22:42  
 Sample : 800ug/L GAS STD 8/25/21  
 Misc : IS&S 6/4/21

Vial: 18  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Aug 26 16:18 2021

Quant Results File: MGAS0825.RES

Quant Method : M:\MAX\DATA\210825\MGAS0825.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Thu Aug 26 16:13:10 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260\_081021

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.21	TIC	288929	25.00	ppb	0.00
3) Chlorobenzene-D5 (IS)	11.75	TIC	313031m	25.00	ppb	0.00
4) 1,4-Dichlorobenzene (IS)	10.94	TIC	240514m	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Gasoline C6-C10	7.95	TIC	6580092m	807.60	ppb	100

Quantitation Report


Data File : M:\MAX\DATA\210825\0825M28.D  
Acq On : 25 Aug 21 22:42  
Sample : 800ug/L GAS STD 8/25/21  
Misc : IS&S 6/4/21

Vial: 18  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Aug 26 16:18 2021

Quant Results File: MGAS0825.RES

Method : M:\MAX\DATA\210825\MGAS0825.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Aug 26 16:19:36 2021  
Response via : Initial Calibration



Quantitation Report (QT Reviewed)

Data File : M:\MAX\DATA\210825\0825M29.D  
 Acq On : 25 Aug 21 23:10  
 Sample : 1000ug/L GAS STD 8/25/21  
 Misc : IS&S 6/4/21

Vial: 19  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Aug 26 16:19 2021

Quant Results File: MGAS0825.RES

Quant Method : M:\MAX\DATA\210825\MGAS0825.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Thu Aug 26 16:13:10 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260\_081021

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.21	TIC	286598	25.00	ppb	0.00
3) Chlorobenzene-D5 (IS)	11.75	TIC	331346m	25.00	ppb	0.00
4) 1,4-Dichlorobenzene (IS)	10.94	TIC	289883m	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Gasoline C6-C10	8.02	TIC	7278206m	979.10	ppb	100

Quantitation Report


Data File : M:\MAX\DATA\210825\0825M29.D  
Acq On : 25 Aug 21 23:10  
Sample : 1000ug/L GAS STD 8/25/21  
Misc : IS&S 6/4/21

Vial: 19  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Aug 26 16:19 2021

Quant Results File: MGAS0825.RES

Method : M:\MAX\DATA\210825\MGAS0825.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Aug 26 16:19:36 2021  
Response via : Initial Calibration



VOLATILE ORGANIC ANALYSIS  
VOLATILE ORGANIC COMPOUNDS

Form 7

Second Source Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: \_\_\_\_\_

SDG No: \_\_\_\_\_  
Date Analyzed: 8/26/2021  
Instrument: Max  
Initial Cal. Date: 8/25/2021  
Data File: 0825M31.D

	Compound	MEAN	CCRF	%D	%Drift	
1	TMHB Gasoline C6-C10	3.704	1.312	65	TMHBL	12
2						
3						
4						
5						
6						
7						
8						
9						
10						
11						
12						
13						
14						
15						
16						
17						
18						
19						
20						
21						
22						
23						
24						
25						
26						
27						
28						
29						
30						
31						
32						
33						
34						
35						
36						
37						
38						
39						
40	Average			65.0		

Quantitation Report (QT Reviewed)

Data File : M:\MAX\DATA\210825\0825M31.D  
 Acq On : 26 Aug 21 00:06  
 Sample : (SS) 300ug/L GAS STD 8/25/21  
 Misc : IS&S 6/4/21

Vial: 21  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Sep 1 8:52 2021

Quant Results File: MGAS0825.RES

Quant Method : M:\MAX\DATA\210825\MGAS0825.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Thu Aug 26 16:19:36 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260\_081021

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.21	TIC	283312	25.00	ppb	0.00
3) Chlorobenzene-D5 (IS)	11.75	TIC	277458m	25.00	ppb	0.00
4) 1,4-Dichlorobenzene (IS)	10.94	TIC	112772m	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Gasoline C6-C10	7.95	TIC	4459802m	336.84	ppb	100

Quantitation Report


Data File : M:\MAX\DATA\210825\0825M31.D  
Acq On : 26 Aug 21 00:06  
Sample : (SS) 300ug/L GAS STD 8/25/21  
Misc : IS&S 6/4/21

Vial: 21  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Sep 1 8:52 2021

Quant. Results File: MGAS0825.RES

Method : M:\MAX\DATA\210825\MGAS0825.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Aug 26 16:19:36 2021  
Response via : Initial Calibration



VOLATILE ORGANIC ANALYSIS  
VOLATILE ORGANIC COMPOUNDS

Form 6  
Initial Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: \_\_\_\_\_

SDG No: \_\_\_\_\_  
Initial Cal. Date: 10/15/2021  
Instrument: Thor

Initials: \_\_\_\_\_

1015B08.D 1015B09.D 1015B10.D 1015B11.D 1015B12.D 1015B13.D 1015B14.D 1015B15.D 1015B16.D

	Compound	1	2	3	4	5	6	7	8	9	Avg	%RSD	Type	r^2	Q	MRF
1	I Fluorobenzene (IS)															
2	S Dibromofluoromethane(S)	0.2057	0.2053	0.2382	0.2368	0.2600	0.2674	0.2770	0.2740	0.2803	0.25	12	S			
3	S 1,2-DCA-D4(S)	0.2334	0.2245	0.2694	0.2694	0.2847	0.2879	0.3003	0.2924	0.2993	0.27	10	S			
4	I Chlorobenzene-D5 (IS)															
5	S Toluene-D8(S)	0.8654	0.8594	0.9920	1.004	1.092	1.104	1.126	1.135	1.151	1.0	11	S			
6	S 4-Bromofluorobenzene(S)	0.3355	0.3157	0.3645	0.3646	0.4126	0.4221	0.4342	0.4365	0.4353	0.39	12	S			
7	I 1,4-Dichlorobenzene-D (IS)															
8																
9																
10																
11																
12																
13																
14																
15																
16																
17																
18																
19																
20																
21																
22																
23																
24																
25																
26																
27																
28																
29																
30																
31																
32																
33																
34																
35																



Quantitation Report (Not Reviewed)

Data File : M:\THOR\DATA\211015\1015B08.D Vial: 8  
 Acq On : 15 Oct 21 15:28 Operator:  
 Sample : 0.3ug/L VOC STD 10/11/21 Inst : Thor  
 Misc : IS&S 8/15/21 Multiplr: 1.00

Quant Time: Oct 21 10:21 2021 Quant Results File: TSUR05.RES

Quant Method : M:\THOR\DATA\211015\TSUR05.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Sat Oct 16 08:16:30 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.34	96	680673	25.00	ppb	0.00
4) Chlorobenzene-D5 (IS)	9.81	117	559947	25.00	ppb	0.00
7) 1,4-Dichlorobenzene-D (IS)	12.37	152	325659	25.00	ppb	0.00
<b>System Monitoring Compounds</b>						
2) Dibromofluoromethane(S)	5.49	111	28123	4.14	ppb	0.00
Spiked Amount	25.000		Recovery	=	16.568%	
3) 1,2-DCA-D4(S)	5.91	65	31890	4.28	ppb	0.00
Spiked Amount	25.000		Recovery	=	17.132%	
5) Toluene-D8(S)	8.22	98	97049	4.18	ppb	0.00
Spiked Amount	25.000		Recovery	=	16.720%	
6) 4-Bromofluorobenzene(S)	11.11	95	37603	4.29	ppb	0.00
Spiked Amount	25.000		Recovery	=	17.164%	

Target Compounds Qvalue

Quantitation Report


Data File : M:\THOR\DATA\211015\1015B08.D  
Acq On : 15 Oct 21 15:28  
Sample : 0.3ug/L VOC STD 10/11/21  
Misc : IS&S 8/15/21

Vial: 8  
Operator:  
Inst : Thor  
Multiplr: 1.00

Quant Time: Oct 21 10:21 2021

Quant Results File: TSUR05.RES

Method : M:\THOR\DATA\211015\TSUR05.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Sat Oct 16 08:16:30 2021  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data File : M:\THOR\DATA\211015\1015B09.D Vial: 9  
 Acq On : 15 Oct 21 15:53 Operator:  
 Sample : 0.5ug/L VOC STD 10/11/21 Inst : Thor  
 Misc : IS&S 8/15/21 Multiplr: 1.00

Quant Time: Oct 21 10:21 2021 Quant Results File: TSUR05.RES

Quant Method : M:\THOR\DATA\211015\TSUR05.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Sat Oct 16 08:16:30 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.35	96	679554	25.00	ppb	0.00
4) Chlorobenzene-D5 (IS)	9.81	117	563117	25.00	ppb	0.00
7) 1,4-Dichlorobenzene-D (IS)	12.37	152	329003	25.00	ppb	0.00
<b>System Monitoring Compounds</b>						
2) Dibromofluoromethane(S)	5.50	111	27927	4.12	ppb	0.00
Spiked Amount	25.000		Recovery	=	16.476%	
3) 1,2-DCA-D4(S)	5.91	65	30593	4.12	ppb	0.00
Spiked Amount	25.000		Recovery	=	16.464%	
5) Toluene-D8(S)	8.22	98	96877	4.15	ppb	0.00
Spiked Amount	25.000		Recovery	=	16.596%	
6) 4-Bromofluorobenzene(S)	11.11	95	35564	4.04	ppb	0.00
Spiked Amount	25.000		Recovery	=	16.144%	

Target Compounds Qvalue

Quantitation Report


Data File : M:\THOR\DATA\211015\1015B09.D  
Acq On : 15 Oct 21 15:53  
Sample : 0.5ug/L VOC STD 10/11/21  
Misc : IS&S 8/15/21

Vial: 9  
Operator:  
Inst : Thor  
Multiplr: 1.00

Quant Time: Oct 21 10:21 2021

Quant Results File: TSUR05.RES

Method : M:\THOR\DATA\211015\TSUR05.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Sat Oct 16 08:16:30 2021  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data File : M:\THOR\DATA\211015\1015B10.D Vial: 10  
 Acq On : 15 Oct 21 16:18 Operator:  
 Sample : 1ug/L VOC STD 10/11/21 Inst : Thor  
 Misc : IS&S 8/15/21 Multiplr: 1.00

Quant Time: Oct 21 10:21 2021 Quant Results File: TSUR05.RES

Quant Method : M:\THOR\DATA\211015\TSUR05.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Sat Oct 16 08:16:30 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.34	96	671281	25.00	ppb	0.00
4) Chlorobenzene-D5 (IS)	9.81	117	560760	25.00	ppb	0.00
7) 1,4-Dichlorobenzene-D (IS)	12.37	152	331921	25.00	ppb	0.00
<b>System Monitoring Compounds</b>						
2) Dibromofluoromethane(S)	5.49	111	64105	9.57	ppb	0.00
Spiked Amount	25.000		Recovery	=	38.292%	
3) 1,2-DCA-D4(S)	5.91	65	72388	9.86	ppb	0.00
Spiked Amount	25.000		Recovery	=	39.432%	
5) Toluene-D8(S)	8.22	98	222754	9.58	ppb	0.00
Spiked Amount	25.000		Recovery	=	38.324%	
6) 4-Bromofluorobenzene(S)	11.11	95	81809	9.32	ppb	0.00
Spiked Amount	25.000		Recovery	=	37.292%	

Target Compounds Qvalue

Quantitation Report


Data File : M:\THOR\DATA\211015\1015B10.D  
Acq On : 15 Oct 21 16:18  
Sample : 1ug/L VOC STD 10/11/21  
Misc : IS&S 8/15/21

Vial: 10  
Operator:  
Inst : Thor  
Multiplr: 1.00

Quant Time: Oct 21 10:21 2021

Quant Results File: TSUR05.RES

Method : M:\THOR\DATA\211015\TSUR05.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Sat Oct 16 08:16:30 2021  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data File : M:\THOR\DATA\211015\1015B11.D Vial: 11  
 Acq On : 15 Oct 21 16:43 Operator:  
 Sample : 2ug/L VOC STD 10/11/21 Inst : Thor  
 Misc : IS&S 8/15/21 Multiplr: 1.00

Quant Time: Oct 21 10:21 2021 Quant Results File: TSUR05.RES

Quant Method : M:\THOR\DATA\211015\TSUR05.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Sat Oct 16 08:16:30 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.34	96	672705	25.00	ppb	0.00
4) Chlorobenzene-D5 (IS)	9.81	117	564069	25.00	ppb	0.00
7) 1,4-Dichlorobenzene-D (IS)	12.37	152	332627	25.00	ppb	0.00
System Monitoring Compounds						
2) Dibromofluoromethane(S)	5.49	111	63844	9.51	ppb	0.00
Spiked Amount	25.000		Recovery	=	38.052%	
3) 1,2-DCA-D4(S)	5.91	65	72709	9.88	ppb	0.00
Spiked Amount	25.000		Recovery	=	39.524%	
5) Toluene-D8(S)	8.22	98	226709	9.69	ppb	0.00
Spiked Amount	25.000		Recovery	=	38.776%	
6) 4-Bromofluorobenzene(S)	11.11	95	82308	9.32	ppb	0.00
Spiked Amount	25.000		Recovery	=	37.296%	

Target Compounds Qvalue

Quantitation Report


Data File : M:\THOR\DATA\211015\1015B11.D  
Acq On : 15 Oct 21 16:43  
Sample : 2ug/L VOC STD 10/11/21  
Misc : IS&S 8/15/21

Vial: 11  
Operator:  
Inst : Thor  
Multiplr: 1.00

Quant Time: Oct 21 10:21 2021

Quant Results File: TSUR05.RES

Method : M:\THOR\DATA\211015\TSUR05.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Sat Oct 16 08:16:30 2021  
Response via : Initial Calibration





Quantitation Report (Not Reviewed)

Data File : M:\THOR\DATA\211015\1015B12.D Vial: 12  
 Acq On : 15 Oct 21 17:07 Operator:  
 Sample : 5ug/L VOC STD 10/11/21 Inst : Thor  
 Misc : IS&S 8/15/21 Multiplr: 1.00

Quant Time: Oct 21 10:21 2021 Quant Results File: TSUR05.RES

Quant Method : M:\THOR\DATA\211015\TSUR05.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Sat Oct 16 08:16:30 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.34	96	681979	25.00	ppb	0.00
4) Chlorobenzene-D5 (IS)	9.81	117	567101	25.00	ppb	0.00
7) 1,4-Dichlorobenzene-D (IS)	12.37	152	339388	25.00	ppb	0.00
System Monitoring Compounds						
2) Dibromofluoromethane(S)	5.49	111	177562	26.10	ppb	0.00
Spiked Amount	25.000		Recovery	=	104.396%	
3) 1,2-DCA-D4(S)	5.91	65	194536	26.08	ppb	0.00
Spiked Amount	25.000		Recovery	=	104.308%	
5) Toluene-D8(S)	8.22	98	620031	26.37	ppb	0.00
Spiked Amount	25.000		Recovery	=	105.480%	
6) 4-Bromofluorobenzene(S)	11.11	95	234125	26.38	ppb	0.00
Spiked Amount	25.000		Recovery	=	105.528%	

Target Compounds Qvalue

Quantitation Report


Data File : M:\THOR\DATA\211015\1015B12.D  
Acq On : 15 Oct 21 17:07  
Sample : 5ug/L VOC STD 10/11/21  
Misc : IS&S 8/15/21

Vial: 12  
Operator:  
Inst : Thor  
Multiplr: 1.00

Quant Time: Oct 21 10:21 2021

Quant Results File: TSUR05.RES

Method : M:\THOR\DATA\211015\TSUR05.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Sat Oct 16 08:16:30 2021  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data File : M:\THOR\DATA\211015\1015B13.D Vial: 13  
 Acq On : 15 Oct 21 17:32 Operator:  
 Sample : 10ug/L VOC STD 10/11/21 Inst : Thor  
 Misc : IS&S 8/15/21 Multiplr: 1.00

Quant Time: Oct 21 10:21 2021 Quant Results File: TSUR05.RES

Quant Method : M:\THOR\DATA\211015\TSUR05.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Sat Oct 16 08:16:30 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.35	96	674780	25.00	ppb	0.00
4) Chlorobenzene-D5 (IS)	9.81	117	569625	25.00	ppb	0.00
7) 1,4-Dichlorobenzene-D (IS)	12.37	152	346728	25.00	ppb	0.00
System Monitoring Compounds						
2) Dibromofluoromethane(S)	5.49	111	180637	26.83	ppb	0.00
Spiked Amount	25.000		Recovery	=	107.336%	
3) 1,2-DCA-D4(S)	5.91	65	194487	26.35	ppb	0.00
Spiked Amount	25.000		Recovery	=	105.396%	
5) Toluene-D8(S)	8.22	98	629134	26.64	ppb	0.00
Spiked Amount	25.000		Recovery	=	106.552%	
6) 4-Bromofluorobenzene(S)	11.11	95	240516	26.98	ppb	0.00
Spiked Amount	25.000		Recovery	=	107.928%	

Target Compounds Qvalue

Quantitation Report


Data File : M:\THOR\DATA\211015\1015B13.D  
Acq On : 15 Oct 21 17:32  
Sample : 10ug/L VOC STD 10/11/21  
Misc : IS&S 8/15/21

Vial: 13  
Operator:  
Inst : Thor  
Multiplr: 1.00

Quant Time: Oct 21 10:21 2021

Quant Results File: TSUR05.RES

Method : M:\THOR\DATA\211015\TSUR05.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Sat Oct 16 08:16:30 2021  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data File : M:\THOR\DATA\211015\1015B14.D Vial: 14  
 Acq On : 15 Oct 21 17:57 Operator:  
 Sample : 20ug/L VOC STD 10/11/21 Inst : Thor  
 Misc : IS&S 8/15/21 Multiplr: 1.00

Quant Time: Oct 21 10:21 2021 Quant Results File: TSUR05.RES

Quant Method : M:\THOR\DATA\211015\TSUR05.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Sat Oct 16 08:16:30 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.34	96	680678	25.00	ppb	0.00
4) Chlorobenzene-D5 (IS)	9.81	117	578119	25.00	ppb	0.00
7) 1,4-Dichlorobenzene-D (IS)	12.37	152	350553	25.00	ppb	0.00
System Monitoring Compounds						
2) Dibromofluoromethane(S)	5.49	111	377523	55.60	ppb	0.00
Spiked Amount	25.000		Recovery	=	222.384%	
3) 1,2-DCA-D4(S)	5.91	65	409169	54.95	ppb	0.00
Spiked Amount	25.000		Recovery	=	219.816%	
5) Toluene-D8(S)	8.22	98	1302348	54.33	ppb	0.00
Spiked Amount	25.000		Recovery	=	217.332%	
6) 4-Bromofluorobenzene(S)	11.11	95	502182	55.51	ppb	0.00
Spiked Amount	25.000		Recovery	=	222.032%	

Target Compounds Qvalue

Quantitation Report


Data File : M:\THOR\DATA\211015\1015B14.D  
Acq On : 15 Oct 21 17:57  
Sample : 20ug/L VOC STD 10/11/21  
Misc : IS&S 8/15/21

Vial: 14  
Operator:  
Inst : Thor  
Multiplr: 1.00

Quant Time: Oct 21 10:21 2021

Quant Results File: TSUR05.RES

Method : M:\THOR\DATA\211015\TSUR05.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Sat Oct 16 08:16:30 2021  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data File : M:\THOR\DATA\211015\1015B15.D Vial: 15  
 Acq On : 15 Oct 21 18:22 Operator:  
 Sample : 40ug/L VOC STD 10/11/21 Inst : Thor  
 Misc : IS&S 8/15/21 Multiplr: 1.00

Quant Time: Oct 21 10:21 2021 Quant Results File: TSUR05.RES

Quant Method : M:\THOR\DATA\211015\TSUR05.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Sat Oct 16 08:16:30 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.34	96	695207	25.00	ppb	0.00
4) Chlorobenzene-D5 (IS)	9.81	117	585054	25.00	ppb	0.00
7) 1,4-Dichlorobenzene-D (IS)	12.37	152	347524	25.00	ppb	0.00
System Monitoring Compounds						
2) Dibromofluoromethane(S)	5.49	111	381406	54.99	ppb	0.00
Spiked Amount				25.000		
					Recovery =	219.976%
3) 1,2-DCA-D4(S)	5.91	65	407840	53.63	ppb	0.00
Spiked Amount				25.000		
					Recovery =	214.524%
5) Toluene-D8(S)	8.22	98	1328991	54.79	ppb	0.00
Spiked Amount				25.000		
					Recovery =	219.148%
6) 4-Bromofluorobenzene(S)	11.11	95	510731	55.78	ppb	0.00
Spiked Amount				25.000		
					Recovery =	223.136%

Target Compounds Qvalue

Quantitation Report


Data File : M:\THOR\DATA\211015\1015B15.D  
Acq On : 15 Oct 21 18:22  
Sample : 40ug/L VOC STD 10/11/21  
Misc : IS&S 8/15/21

Vial: 15  
Operator:  
Inst : Thor  
Multiplr: 1.00

Quant Time: Oct 21 10:21 2021

Quant Results File: TSUR05.RES

Method : M:\THOR\DATA\211015\TSUR05.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Sat Oct 16 08:16:30 2021  
Response via : Initial Calibration



512 of 591



Quantitation Report (Not Reviewed)

Data File : M:\THOR\DATA\211015\1015B16.D Vial: 16  
 Acq On : 15 Oct 21 18:47 Operator:  
 Sample : 100ug/L VOC STD 10/11/21 Inst : Thor  
 Misc : IS&S 8/15/21 Multiplr: 1.00

Quant Time: Oct 21 10:21 2021 Quant Results File: TSUR05.RES

Quant Method : M:\THOR\DATA\211015\TSUR05.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Sat Oct 16 08:16:30 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.34	96	702856	25.00	ppb	0.00
4) Chlorobenzene-D5 (IS)	9.81	117	584886	25.00	ppb	0.00
7) 1,4-Dichlorobenzene-D (IS)	12.37	152	346746	25.00	ppb	0.00
System Monitoring Compounds						
2) Dibromofluoromethane(S)	5.49	111	788862	112.51	ppb	0.00
Spiked Amount	25.000		Recovery	= 450.024%		
3) 1,2-DCA-D4(S)	5.91	65	844481	109.84	ppb	0.00
Spiked Amount	25.000		Recovery	= 439.360%		
5) Toluene-D8(S)	8.22	98	2692804	111.04	ppb	0.00
Spiked Amount	25.000		Recovery	= 444.164%		
6) 4-Bromofluorobenzene(S)	11.11	95	1018320	111.26	ppb	0.00
Spiked Amount	25.000		Recovery	= 445.028%		

Target Compounds Qvalue

Quantitation Report


Data File : M:\THOR\DATA\211015\1015B16.D  
Acq On : 15 Oct 21 18:47  
Sample : 100ug/L VOC STD 10/11/21  
Misc : IS&S 8/15/21

Vial: 16  
Operator:  
Inst : Thor  
Multiplr: 1.00

Quant Time: Oct 21 10:21 2021

Quant Results File: TSUR05.RES

Method : M:\THOR\DATA\211015\TSUR05.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Sat Oct 16 08:16:30 2021  
Response via : Initial Calibration



VOLATILE ORGANIC ANALYSIS  
VOLATILE ORGANIC COMPOUNDS

Form 6  
Initial Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: \_\_\_\_\_

SDG No: \_\_\_\_\_  
Initial Cal. Date: 10/15/2021  
Instrument: Thor

Initials: \_\_\_\_\_

1015B19.D    1015B20.D    1015B21.D    1015B22.D    1015B23.D    1015B24.D    1015B25.D

	Compound	1	2	3	4	5	6	7				Avg	%RSD	Type	r <sup>2</sup>	Q	MRF
1	I Fluorobenzene (IS)																
2	TMHBI Gasoline C6-C10	12.0	5.051	2.805	1.292	0.8713	0.8571	0.7688				3.4	122	TMHB	0.995		
3	I Chlorobenzene-D5 (IS)																
4	I 1,4-Dichlorobenzene-D (IS)																
5																	
6																	
7																	
8																	
9																	
10																	
11																	
12																	
13																	
14																	
15																	
16																	
17																	
18																	
19																	
20																	
21																	
22																	
23																	
24																	
25																	
26																	
27																	
28																	
29																	
30																	
31																	
32																	
33																	
34																	
35																	

Data File : M:\THOR\DATA\211015\1015B19.D Vial: 19  
 Acq On : 15 Oct 21 20:01 Operator:  
 Sample : 20 ug/L GAS STD 10/15/21 Inst : Thor  
 Misc : IS&S 8/15/21 Multiplr: 1.00

Quant Time: Oct 16 10:36 2021 Quant Results File: TGAS1015.RES

Quant Method : M:\THOR\DATA\211015\TGAS1015.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Sat Oct 16 10:34:55 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
1) Fluorobenzene (IS)	6.34	TIC	703619	25.00 ppb	0.00
3) Chlorobenzene-D5 (IS)	12.37	TIC	998740	25.00 ppb	0.00
4) 1,4-Dichlorobenzene-D (IS)	12.37	TIC	998740	25.00 ppb	0.00

System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc Units	Qvalue
2) Gasoline C6-C10	8.18	TIC	6778242m	35.65 ppb	100

Quantitation Report


Data File : M:\THOR\DATA\211015\1015B19.D  
Acq On : 15 Oct 21 20:01  
Sample : 20 ug/L GAS STD 10/15/21  
Misc : IS&S 8/15/21

Vial: 19  
Operator:  
Inst : Thor  
Multiplr: 1.00

Quant Time: Oct 16 10:36 2021

Quant Results File: TGAS1015.RES

Method : M:\THOR\DATA\211015\TGAS1015.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Oct 21 10:04:41 2021  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data File : M:\THOR\DATA\211015\1015B20.D Vial: 20  
 Acq On : 15 Oct 21 20:26 Operator:  
 Sample : 50 ug/L GAS STD 10/15/21 Inst : Thor  
 Misc : IS&S 8/15/21 Multiplr: 1.00

Quant Time: Oct 16 10:36 2021 Quant Results File: TGAS1015.RES

Quant Method : M:\THOR\DATA\211015\TGAS1015.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Sat Oct 16 10:34:55 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc Units	Dev(Min)
1) Fluorobenzene (IS)	6.34	TIC	706391	25.00 ppb	0.00
3) Chlorobenzene-D5 (IS)	12.37	TIC	993334	25.00 ppb	0.00
4) 1,4-Dichlorobenzene-D (IS)	12.37	TIC	993334	25.00 ppb	0.00

System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc Units	Qvalue
2) Gasoline C6-C10	8.18	TIC	7136092m	54.59 ppb	100

Quantitation Report


Data File : M:\THOR\DATA\211015\1015B20.D  
Acq On : 15 Oct 21 20:26  
Sample : 50 ug/L GAS STD 10/15/21  
Misc : IS&S 8/15/21

Vial: 20  
Operator:  
Inst : Thor  
Multiplr: 1.00

Quant Time: Oct 16 10:36 2021

Quant Results File: TGAS1015.RES

Method : M:\THOR\DATA\211015\TGAS1015.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Oct 21 10:04:41 2021  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data File : M:\THOR\DATA\211015\1015B21.D Vial: 21  
 Acq On : 15 Oct 21 20:51 Operator:  
 Sample : 100 ug/L GAS STD 10/15/21 Inst : Thor  
 Misc : IS&S 8/15/21 Multiplr: 1.00

Quant Time: Oct 16 10:36 2021 Quant Results File: TGAS1015.RES

Quant Method : M:\THOR\DATA\211015\TGAS1015.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Sat Oct 16 10:34:55 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.34	TIC	696215	25.00	ppb	0.00
3) Chlorobenzene-D5 (IS)	12.37	TIC	986300	25.00	ppb	0.00
4) 1,4-Dichlorobenzene-D (IS)	12.37	TIC	986300	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Gasoline C6-C10	8.18	TIC	7812597m	99.83	ppb	100



Quantitation Report


Data File : M:\THOR\DATA\211015\1015B21.D  
Acq On : 15 Oct 21 20:51  
Sample : 100 ug/L GAS STD 10/15/21  
Misc : IS&S 8/15/21

Vial: 21  
Operator:  
Inst : Thor  
Multiplr: 1.00

Quant Time: Oct 16 10:36 2021

Quant Results File: TGAS1015.RES

Method : M:\THOR\DATA\211015\TGAS1015.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Oct 21 10:04:41 2021  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data File : M:\THOR\DATA\211015\1015B22.D Vial: 22  
 Acq On : 15 Oct 21 21:16 Operator:  
 Sample : 300 ug/L GAS STD 10/15/21 Inst : Thor  
 Misc : IS&S 8/15/21 Multiplr: 1.00

Quant Time: Oct 16 10:36 2021 Quant Results File: TGAS1015.RES

Quant Method : M:\THOR\DATA\211015\TGAS1015.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Sat Oct 16 10:34:55 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.35	TIC	679855	25.00	ppb	0.00
3) Chlorobenzene-D5 (IS)	12.37	TIC	983747	25.00	ppb	0.00
4) 1,4-Dichlorobenzene-D (IS)	12.37	TIC	983747	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Gasoline C6-C10	8.18	TIC	10541129m	272.94	ppb	100

Quantitation Report


Data File : M:\THOR\DATA\211015\1015B22.D  
Acq On : 15 Oct 21 21:16  
Sample : 300 ug/L GAS STD 10/15/21  
Misc : IS&S 8/15/21

Vial: 22  
Operator:  
Inst : Thor  
Multiplr: 1.00

Quant Time: Oct 16 10:36 2021

Quant Results File: TGAS1015.RES

Method : M:\THOR\DATA\211015\TGAS1015.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Oct 21 10:04:41 2021  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data File : M:\THOR\DATA\211015\1015B23.D Vial: 23  
 Acq On : 15 Oct 21 21:40 Operator:  
 Sample : 600 ug/L GAS STD 10/15/21 Inst : Thor  
 Misc : IS&S 8/15/21 Multiplr: 1.00

Quant Time: Oct 16 10:36 2021 Quant Results File: TGAS1015.RES

Quant Method : M:\THOR\DATA\211015\TGAS1015.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Sat Oct 16 10:34:55 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.34	TIC	686558	25.00	ppb	0.00
3) Chlorobenzene-D5 (IS)	12.37	TIC	982427	25.00	ppb	0.00
4) 1,4-Dichlorobenzene-D (IS)	12.37	TIC	982427	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Gasoline C6-C10	8.18	TIC	14357235m	491.45	ppb	100

Quantitation Report


Data File : M:\THOR\DATA\211015\1015B23.D  
Acq On : 15 Oct 21 21:40  
Sample : 600 ug/L GAS STD 10/15/21  
Misc : IS&S 8/15/21

Vial: 23  
Operator:  
Inst : Thor  
Multiplr: 1.00

Quant Time: Oct 16 10:36 2021

Quant Results File: TGAS1015.RES

Method : M:\THOR\DATA\211015\TGAS1015.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Oct 21 10:04:41 2021  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data File : M:\THOR\DATA\211015\1015B24.D Vial: 24  
 Acq On : 15 Oct 21 22:05 Operator:  
 Sample : 800 ug/L GAS STD 10/15/21 Inst : Thor  
 Misc : IS&S 8/15/21 Multiplr: 1.00

Quant Time: Oct 16 10:36 2021 Quant Results File: TGAS1015.RES

Quant Method : M:\THOR\DATA\211015\TGAS1015.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Sat Oct 16 10:34:55 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.34	TIC	681758	25.00	ppb	0.00
3) Chlorobenzene-D5 (IS)	12.37	TIC	1001978	25.00	ppb	0.00
4) 1,4-Dichlorobenzene-D (IS)	12.37	TIC	1001978	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Gasoline C6-C10	8.18	TIC	18699305m	754.80	ppb	100

Quantitation Report


Data File : M:\THOR\DATA\211015\1015B24.D  
Acq On : 15 Oct 21 22:05  
Sample : 800 ug/L GAS STD 10/15/21  
Misc : IS&S 8/15/21

Vial: 24  
Operator:  
Inst : Thor  
Multiplr: 1.00

Quant Time: Oct 16 10:36 2021

Quant Results File: TGAS1015.RES

Method : M:\THOR\DATA\211015\TGAS1015.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Oct 21 10:04:41 2021  
Response via : Initial Calibration



Quantitation Report (Not Reviewed)

Data File : M:\THOR\DATA\211015\1015B25.D Vial: 25  
 Acq On : 15 Oct 21 22:30 Operator:  
 Sample : 1000 ug/L GAS STD 10/15/21 Inst : Thor  
 Misc : IS&S 8/15/21 Multiplr: 1.00

Quant Time: Oct 16 10:36 2021 Quant Results File: TGAS1015.RES

Quant Method : M:\THOR\DATA\211015\TGAS1015.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Sat Oct 16 10:34:55 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.35	TIC	688634	25.00	ppb	0.00
3) Chlorobenzene-D5 (IS)	12.37	TIC	980725	25.00	ppb	0.00
4) 1,4-Dichlorobenzene-D (IS)	12.37	TIC	980725	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Gasoline C6-C10	8.18	TIC	21177421m	889.16	ppb	100



Quantitation Report


Data File : M:\THOR\DATA\211015\1015B25.D  
Acq On : 15 Oct 21 22:30  
Sample : 1000 ug/L GAS STD 10/15/21  
Misc : IS&S 8/15/21

Vial: 25  
Operator:  
Inst : Thor  
Multiplr: 1.00

Quant Time: Oct 16 10:36 2021

Quant Results File: TGAS1015.RES

Method : M:\THOR\DATA\211015\TGAS1015.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Oct 21 10:04:41 2021  
Response via : Initial Calibration



VOLATILE ORGANIC ANALYSIS  
VOLATILE ORGANIC COMPOUNDS

Form 7

Second Source Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Date Analyzed: 10/15/2021  
Instrument: Thor  
Initial Cal. Date: 10/15/2021  
Data File: 1015B27.D

	Compound	MEAN	CCRF	%D	%Drift
1	TMHB Gasoline C6-C10	3.384	1.264	63	TMHBL 5.6
2					
3					
4					
5					
6					
7					
8					
9					
10					
11					
12					
13					
14					
15					
16					
17					
18					
19					
20					
21					
22					
23					
24					
25					
26					
27					
28					
29					
30					
31					
32					
33					
34					
35					
36					
37					
38					
39					
40	Average			63.0	

Quantitation Report (QT Reviewed)

Data File : M:\THOR\DATA\211015\1015B27.D Vial: 27  
 Acq On : 15 Oct 21 23:19 Operator:  
 Sample : (SS) 300ug/L GAS STD 10/15/21 Inst : Thor  
 Misc : IS&S 8/15/21 Multiplr: 1.00

Quant Time: Oct 18 7:16 2021

Quant Results File: TGAS1015.RES

Quant Method : M:\THOR\DATA\211015\TGAS1015.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Mon Oct 18 08:12:38 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.34	TIC	686562	25.00	ppb	0.00
3) Chlorobenzene-D5 (IS)	12.37	TIC	957857	25.00	ppb	0.00
4) 1,4-Dichlorobenzene-D (IS)	12.37	TIC	957857	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Gasoline C6-C10	9.81	TIC	10414158m	283.32	ppb	100



VOLATILE ORGANIC ANALYSIS  
VOLATILE ORGANIC COMPOUNDS

Form 7

Continuing Calibration

Lab Name: APPL, Inc.

SDG No: \_\_\_\_\_

Case No: \_\_\_\_\_

Date Analyzed: 11/15/2021

Matrix: Water

Instrument: Max

Initial Cal. Date: 8/25/2021

Data File: 1115M05.D

	Compound	MEAN	CCRF	%D	%Drift
1	Fluorobenzene (IS)	ISTD			
2	TMHB Gasoline C6-C10	3.704	1.282	65	TMHBL 4.3
3	TMHB Chlorobenzene-D5 (IS)	ISTD			TMHB
4	TMHB 1,4-Dichlorobenzene (IS)	ISTD			TMHB
5					
6					
7					
8					
9					
10					
11					
12					
13					
14					
15					
16					
17					
18					
19					
20					
21					
22					
23					
24					
25					
26					
27					
28					
29					
30					
31					
32					
33					
34					
35					
36					
37					
38					
39					
40	Average			65.0	

VOLATILE ORGANIC ANALYSIS  
VOLATILE ORGANIC COMPOUNDS

Form 7

Continuing Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Date Analyzed: 11/19/2021  
Instrument: Thor  
Initial Cal. Date: 10/15/2021  
Data File: 1119T34.D

	Compound	MEAN	CCRF	%D	%Drift
1	I Fluorobenzene (IS)	ISTD			I
2	TMHB Gasoline C6-C10	3.384	1.280	62	TMHBL 2.6
3	I Chlorobenzene-D5 (IS)	ISTD			I
4	I 1,4-Dichlorobenzene-D (IS)	ISTD			I
5					
6					
7					
8					
9					
10					
11					
12					
13					
14					
15					
16					
17					
18					
19					
20					
21					
22					
23					
24					
25					
26					
27					
28					
29					
30					
31					
32					
33					
34					
35					
36					
37					
38					
39					
40	Average			62.0	

Data File : M:\MAX\DATA\211111\1115M05.D  
 Acq On : 15 Nov 21 10:25  
 Sample : 211115A CCV 300ug/L  
 Misc : IS&S 8/4/21

Vial: 5  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 15 10:50 2021

Quant Results File: MGAS0825.RES

Quant Method : M:\MAX\DATA\210922\MGAS0825.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Thu Aug 26 16:19:36 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.38	TIC	463816	25.00	ppb	0.17
3) Chlorobenzene-D5 (IS)	11.75	TIC	1158760m	25.00	ppb	0.00
4) 1,4-Dichlorobenzene (IS)	10.94	TIC	126352m	25.00	ppb	0.00

#### System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Gasoline C6-C10	8.08	TIC	7136217m	312.91	ppb	100

Quantitation Report (Not Reviewed)

Data File : M:\MAX\DATA\211111\1115M05.D	Vial: 5
Acq On : 15 Nov 21 10:25	Operator: LP, DG, CH
Sample : 211115A CCV 300ug/L	Inst : Max
Misc : IS&S 8/4/21	Multiplr: 1.00

Quant Time: Nov 22 16:29 2021 Quant Results File: M0825SUR.RES

Quant Method : M:\MAX\DATA\210922\M0825SUR.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Thu Aug 26 11:16:48 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.38	96	379420	25.00	ppb	0.17
4) Chlorobenzene-D5 (IS)	9.53	117	348435	25.00	ppb	0.12
7) 1,4-Dichlorobenzene-D (IS)	11.85	152	216125	25.00	ppb	0.11
<b>System Monitoring Compounds</b>						
2) Dibromofluoromethane (S)	5.60	111	128636	28.11	ppb	0.18
Spiked Amount						
			Recovery	=		112.448%
3) 1,2-DCA-D4 (S)	5.99	65	86128	28.64	ppb	0.17
Spiked Amount						
			Recovery	=		114.568%
5) Toluene-D8 (S)	8.08	98	410630	25.13	ppb	0.13
Spiked Amount						
			Recovery	=		100.524%
6) 4-Bromofluorobenzene (S)	10.71	95	156631	24.57	ppb	0.11
Spiked Amount						
			Recovery	=		98.280%

Target Compounds Qvalue



Quantitation Report


Data File : M:\MAX\DATA\211111\1115M05.D  
Acq On : 15 Nov 21 10:25  
Sample : 211115A CCV 300ug/L  
Misc : IS&S 8/4/21

Vial: 5  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Nov 15 10:50 2021

Quant Results File: MGAS0825.RES

Method : M:\MAX\DATA\210922\MGAS0825.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Aug 26 16:19:36 2021  
Response via : Initial Calibration



VOLATILE ORGANIC ANALYSIS  
VOLATILE ORGANIC COMPOUNDS

Form 7

Continuing Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Date Analyzed: 11/19/2021  
Instrument: Thor  
Initial Cal. Date: 10/15/2021  
Data File: 1119T34.D

		Compound	MEAN	CCRF	%D	%Drift	
1	I	Fluorobenzene (IS)	ISTD			I	
2	S	Dibromofluoromethane(S)	0.2494	0.3122	25	S	*NT
3	S	1,2-DCA-D4(S)	0.2735	0.3421	25	S	*NT
4	I	Chlorobenzene-D5 (IS)	ISTD			I	
5	S	Toluene-D8(S)	1.037	1.011	2.5	S	
6	S	4-Bromofluorobenzene(S)	0.3912	0.4114	5.2	S	
7	I	1,4-Dichlorobenzene-D (IS)	ISTD			I	
8							
9							
10							
11							
12							
13							
14							
15							
16							
17							
18							
19							
20							
21							
22							
23							
24							
25							
26							
27							
28							
29							
30							
31							
32							
33							
34							
35							
36							
37							
38							
39							
40		Average			14.4		

Data File : M:\THOR\DATA\211111\1119T34.D Vial: 34  
 Acq On : 19 Nov 21 23:25 Operator:  
 Sample : 211119B CCV 300ug/L Inst : Thor  
 Misc : IS&S 8/15/21 Multiplr: 1.00

Quant Time: Nov 22 12:43 2021 Quant Results File: TGAS1015.RES

Quant Method : M:\THOR\DATA\211015\TGAS1015.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Thu Oct 21 10:04:41 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.34	TIC	253530	25.00	ppb	0.00
3) Chlorobenzene-D5 (IS)	12.37	TIC	499137	25.00	ppb	0.00
4) 1,4-Dichlorobenzene-D (IS)	12.37	TIC	499137	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Gasoline C6-C10	11.11	TIC	3894398m	292.11	ppb	100

Data File : M:\THOR\DATA\211111\1119T34.D  
 Acq On : 19 Nov 21 23:25  
 Sample : 211119B CCV 300ug/L  
 Misc : IS&S 8/15/21

Vial: 34  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 22 12:51 2021

Quant Results File: TSUR05.RES

Quant Method : M:\THOR\DATA\211015\TSUR05.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Sun Oct 24 10:14:29 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.34	96	255806	25.00	ppb	0.00
5) Chlorobenzene-D5 (IS)	9.81	117	254174	25.00	ppb	0.00
8) 1,4-Dichlorobenzene-D (IS)	12.37	152	188865	25.00	ppb	0.00
System Monitoring Compounds						
2) Dibromofluoromethane (S)	5.49	111	79866	31.30	ppb	0.00
Spiked Amount						
						Recovery = 125.184%
3) 1,2-DCA-D4 (S)	5.91	65	87500	31.27	ppb	0.00
Spiked Amount						
						Recovery = 125.080%
6) Toluene-D8 (S)	8.22	98	256958	24.38	ppb	0.00
Spiked Amount						
						Recovery = 97.532%
7) 4-Bromofluorobenzene (S)	11.11	95	104566	26.29	ppb	0.00
Spiked Amount						
						Recovery = 105.156%

Target Compounds

Qvalue

Quantitation Report


Data File : M:\THOR\DATA\211111\1119T34.D  
Acq On : 19 Nov 21 23:25  
Sample : 211119B CCV 300ug/L  
Misc : IS&S 8/15/21

Vial: 34  
Operator:  
Inst : Thor  
Multiplr: 1.00

Quant Time: Nov 22 12:43 2021

Quant Results File: TGAS1015.RES

Method : M:\THOR\DATA\211015\TGAS1015.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Oct 21 10:04:41 2021  
Response via : Initial Calibration



VOLATILE ORGANIC ANALYSIS  
VOLATILE ORGANIC COMPOUNDS

Form 7

Ending Continuing Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Date Analyzed: 11/15/2021  
Instrument: Max  
Initial Cal. Date: 8/25/2021  
Data File: 1115M26.D

	Compound	MEAN	CCRF	%D	%Drift
1	I Fluorobenzene (IS)	ISTD			I
2	TMHB Gasoline C6-C10	3.704	1.283	65	TMHBL 4.6
3	TMHB Chlorobenzene-D5 (IS)	ISTD			TMHB
4	TMHB 1,4-Dichlorobenzene (IS)	ISTD			TMHB
5					
6					
7					
8					
9					
10					
11					
12					
13					
14					
15					
16					
17					
18					
19					
20					
21					
22					
23					
24					
25					
26					
27					
28					
29					
30					
31					
32					
33					
34					
35					
36					
37					
38					
39					
40	Average			65.0	

Data File : M:\MAX\DATA\211111\1115M26.D  
 Acq On : 15 Nov 21 20:21  
 Sample : Ending CCV 300ug/L 11/15/21  
 Misc : IS&S 8/4/21

Vial: 26  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 16 10:18 2021

Quant Results File: MGAS0825.RES

Quant Method : M:\MAX\DATA\210922\MGAS0825.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Thu Aug 26 16:19:36 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.37	TIC	428733	25.00	ppb	0.16
3) Chlorobenzene-D5 (IS)	11.75	TIC	1092850m	25.00	ppb	0.00
4) 1,4-Dichlorobenzene (IS)	10.94	TIC	115781m	25.00	ppb	0.00

#### System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Gasoline C6-C10	8.08	TIC	6602956m	313.93	ppb	100

Data File : M:\MAX\DATA\211111\1115M26.D  
 Acq On : 15 Nov 21 20:21  
 Sample : Ending CCV 300ug/L 11/15/21  
 Misc : IS&S 8/4/21

Vial: 26  
 Operator: LP, DG, CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 22 16:29 2021

Quant Results File: M0825SUR.RES

Quant Method : M:\MAX\DATA\210922\M0825SUR.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Thu Aug 26 11:16:48 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.37	96	363319	25.00	ppb	0.16
4) Chlorobenzene-D5 (IS)	9.53	117	334597	25.00	ppb	0.12
7) 1,4-Dichlorobenzene-D (IS)	11.85	152	210878	25.00	ppb	0.10
<b>System Monitoring Compounds</b>						
2) Dibromofluoromethane(S)	5.60	111	121628	27.76	ppb	0.18
Spiked Amount	25.000		Recovery	=	111.036%	
3) 1,2-DCA-D4 (S)	5.98	65	83040	28.84	ppb	0.17
Spiked Amount	25.000		Recovery	=	115.356%	
5) Toluene-D8 (S)	8.08	98	396557	25.27	ppb	0.13
Spiked Amount	25.000		Recovery	=	101.096%	
6) 4-Bromofluorobenzene(S)	10.70	95	148878	24.32	ppb	0.11
Spiked Amount	25.000		Recovery	=	97.280%	

Target Compounds

Qvalue



Quantitation Report


Data File : M:\MAX\DATA\211111\1115M26.D  
Acq On : 15 Nov 21 20:21  
Sample : Ending CCV 300ug/L 11/15/21  
Misc : IS&S 8/4/21

Vial: 26  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Nov 16 10:18 2021

Quant Results File: MGAS0825.RES

Method : M:\MAX\DATA\210922\MGAS0825.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Aug 26 16:19:36 2021  
Response via : Initial Calibration



VOLATILE ORGANIC ANALYSIS  
VOLATILE ORGANIC COMPOUNDS

Form 7

Ending Continuing Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Date Analyzed: 11/20/2021  
Instrument: Thor  
Initial Cal. Date: 10/15/2021  
Data File: 1119T53.D

	Compound	MEAN	CCRF	%D	%Drift
1	I Fluorobenzene (IS)	ISTD			I
2	TMHB Gasoline C6-C10	3.384	1.319	61	TMHBL 4.6
3	I Chlorobenzene-D5 (IS)	ISTD			I
4	I 1,4-Dichlorobenzene-D (IS)	ISTD			I
5					
6					
7					
8					
9					
10					
11					
12					
13					
14					
15					
16					
17					
18					
19					
20					
21					
22					
23					
24					
25					
26					
27					
28					
29					
30					
31					
32					
33					
34					
35					
36					
37					
38					
39					
40	Average			61.0	

VOLATILE ORGANIC ANALYSIS  
VOLATILE ORGANIC COMPOUNDS

Form 7

Ending Continuing Calibration

Lab Name: APPL, Inc.  
Case No: \_\_\_\_\_  
Matrix: Water

SDG No: \_\_\_\_\_  
Date Analyzed: 11/20/2021  
Instrument: Thor  
Initial Cal. Date: 10/15/2021  
Data File: 1119T53.D

		Compound	MEAN	CCRF	%D	%Drift
1	I	Fluorobenzene (IS)	ISTD			I
2	S	Dibromofluoromethane(S)	0.2494	0.3178	27	S
3	S	1,2-DCA-D4(S)	0.2735	0.3393	24	S
4	I	Chlorobenzene-D5 (IS)	ISTD			I
5	S	Toluene-D8(S)	1.037	0.9963	3.9	S
6	S	4-Bromofluorobenzene(S)	0.3912	0.4028	3.0	S
7	I	1,4-Dichlorobenzene-D (IS)	ISTD			I
8						
9						
10						
11						
12						
13						
14						
15						
16						
17						
18						
19						
20						
21						
22						
23						
24						
25						
26						
27						
28						
29						
30						
31						
32						
33						
34						
35						
36						
37						
38						
39						
40		Average			14.5	

Data File : M:\THOR\DATA\211111\1119T53.D Vial: 53  
 Acq On : 20 Nov 21 7:11 Operator:  
 Sample : Ending CCV 300ug/L 11/19/21 Inst : Thor  
 Misc : IS&S 8/15/21 Multiplr: 1.00

Quant Time: Nov 22 12:47 2021 Quant Results File: TGAS1015.RES

Quant Method : M:\THOR\DATA\211015\TGAS1015.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Thu Oct 21 10:04:41 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.34	TIC	252005	25.00	ppb	0.00
3) Chlorobenzene-D5 (IS)	12.37	TIC	500032	25.00	ppb	0.00
4) 1,4-Dichlorobenzene-D (IS)	12.37	TIC	500032	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Gasoline C6-C10	11.11	TIC	3989776m	313.69	ppb	100

Data File : M:\THOR\DATA\211111\1119T53.D  
 Acq On : 20 Nov 21 7:11  
 Sample : Ending CCV 300ug/L 11/19/21  
 Misc : IS&S 8/15/21

Vial: 53  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 22 12:51 2021

Quant Results File: TSUR05.RES

Quant Method : M:\THOR\DATA\211015\TSUR05.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Sun Oct 24 10:14:29 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.34	96	252847	25.00	ppb	0.00
5) Chlorobenzene-D5 (IS)	9.81	117	261762	25.00	ppb	0.00
8) 1,4-Dichlorobenzene-D (IS)	12.37	152	190196	25.00	ppb	0.00
System Monitoring Compounds						
2) Dibromofluoromethane(S)	5.49	111	80343	31.85	ppb	0.00
Spiked Amount			Recovery	=	127.408%	
3) 1,2-DCA-D4(S)	5.91	65	85783	31.02	ppb	0.00
Spiked Amount			Recovery	=	124.064%	
6) Toluene-D8(S)	8.22	98	260798	24.03	ppb	0.00
Spiked Amount			Recovery	=	96.120%	
7) 4-Bromofluorobenzene(S)	11.11	95	105432	25.74	ppb	0.00
Spiked Amount			Recovery	=	102.952%	

Target Compounds

Qvalue

Quantitation Report


Data File : M:\THOR\DATA\211111\1119T53.D  
Acq On : 20 Nov 21 7:11  
Sample : Ending CCV 300ug/L 11/19/21  
Misc : IS&S 8/15/21

Vial: 53  
Operator:  
Inst : Thor  
Multiplr: 1.00

Quant Time: Nov 22 12:47 2021

Quant Results File: TGAS1015.RES

Method : M:\THOR\DATA\211015\TGAS1015.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Oct 21 10:04:41 2021  
Response via : Initial Calibration



**ORGANICS**  
**Raw Data**

Quantitation Report (QT Reviewed)

Data File : M:\MAX\DATA\211111\1115M12.D  
 Acq On : 15 Nov 21 13:44  
 Sample : BA46114W01  
 Misc : IS&S 8/4/21

Vial: 12  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 22 16:12 2021

Quant Results File: MGAS0825.RE

Quant Method : M:\MAX\DATA\210922\MGAS0825.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Thu Aug 26 16:19:36 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.38	TIC	418451	25.00	ppb	0.16
3) Chlorobenzene-D5 (IS)	11.75	TIC	1095204m	25.00	ppb	0.00
4) 1,4-Dichlorobenzene (IS)	10.94	TIC	12383m	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds Qvalue



Quantitation Report (Not Reviewed)

Data File : M:\MAX\DATA\211111\1115M12.D  
 Acq On : 15 Nov 21 13:44  
 Sample : BA46114W01  
 Misc : IS&S 8/4/21

Vial: 12  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 22 16:26 2021

Quant Results File: M0825SUR.RE

Quant Method : M:\MAX\DATA\210922\M0825SUR.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Thu Aug 26 11:16:48 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.38	96	343693	25.00	ppb	0.16
4) Chlorobenzene-D5 (IS)	9.53	117	329377	25.00	ppb	0.12
7) 1,4-Dichlorobenzene-D (IS)	11.85	152	206728	25.00	ppb	0.11
<b>System Monitoring Compounds</b>						
2) Dibromofluoromethane(S)	5.60	111	120212	29.00	ppb	0.18
Spiked Amount	25.000		Recovery	=	116.008%	
3) 1,2-DCA-D4(S)	5.98	65	82336	30.23	ppb	0.17
Spiked Amount	25.000		Recovery	=	120.912%	
5) Toluene-D8(S)	8.08	98	383609	24.84	ppb	0.13
Spiked Amount	25.000		Recovery	=	99.344%	
6) 4-Bromofluorobenzene(S)	10.71	95	150594	24.99	ppb	0.11
Spiked Amount	25.000		Recovery	=	99.960%	

Target Compounds

Qvalue

Quantitation Report


Data File : M:\MAX\DATA\211111\1115M12.D  
Acq On : 15 Nov 21 13:44  
Sample : BA46114W01  
Misc : IS&S 8/4/21

Vial: 12  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Nov 22 16:12 2021

Quant Results File: MGAS0825.RE

Method : M:\MAX\DATA\210922\MGAS0825.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Aug 26 16:19:36 2021  
Response via : Initial Calibration



Quantitation Report (QT Reviewed)

Data File : M:\MAX\DATA\211111\1115M13.D Vial: 13  
 Acq On : 15 Nov 21 14:12 Operator: LP,DG,CH  
 Sample : BA46115W01 Inst : Max  
 Misc : IS&S 8/4/21 Multiplr: 1.00

Quant Time: Nov 22 16:13 2021 Quant Results File: MGAS0825.RE.

Quant Method : M:\MAX\DATA\210922\MGAS0825.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Thu Aug 26 16:19:36 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.38	TIC	445836	25.00	ppb	0.16
3) Chlorobenzene-D5 (IS)	11.75	TIC	1076481m	25.00	ppb	0.00
4) 1,4-Dichlorobenzene (IS)	10.94	TIC	12590m	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds Qvalue

Data File : M:\MAX\DATA\211111\1115M13.D  
 Acq On : 15 Nov 21 14:12  
 Sample : BA46115W01  
 Misc : IS&S 8/4/21

Vial: 13  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 22 16:26 2021

Quant Results File: M0825SUR.RE

Quant Method : M:\MAX\DATA\210922\M0825SUR.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Thu Aug 26 11:16:48 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.38	96	362468	25.00	ppb	0.16
4) Chlorobenzene-D5 (IS)	9.53	117	339379	25.00	ppb	0.12
7) 1,4-Dichlorobenzene-D (IS)	11.85	152	200988	25.00	ppb	0.11
System Monitoring Compounds						
2) Dibromofluoromethane(S)	5.60	111	127338	29.13	ppb	0.18
Spiked Amount	25.000					
					Recovery =	116.520%
3) 1,2-DCA-D4(S)	5.99	65	86592	30.14	ppb	0.17
Spiked Amount	25.000					
					Recovery =	120.572%
5) Toluene-D8(S)	8.08	98	401175	25.21	ppb	0.13
Spiked Amount	25.000					
					Recovery =	100.832%
6) 4-Bromofluorobenzene(S)	10.71	95	151857	24.46	ppb	0.11
Spiked Amount	25.000					
					Recovery =	97.828%

Target Compounds

Qvalue

Quantitation Report


Data File : M:\MAX\DATA\211111\1115M13.D  
Acq On : 15 Nov 21 14:12  
Sample : BA46115W01  
Misc : IS&S 8/4/21

Vial: 13  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Nov 22 16:13 2021

Quant Results File: MGAS0825.RE;

Method : M:\MAX\DATA\210922\MGAS0825.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Aug 26 16:19:36 2021  
Response via : Initial Calibration



Data File : M:\MAX\DATA\211111\1115M14.D Vial: 14  
 Acq On : 15 Nov 21 14:40 Operator: LP,DG,CH  
 Sample : BA46116W01 Inst : Max  
 Misc : IS&S 8/4/21 Multiplr: 1.00

Quant Time: Nov 22 16:13 2021 Quant Results File: MGAS0825.RE

Quant Method : M:\MAX\DATA\210922\MGAS0825.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Thu Aug 26 16:19:36 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.38	TIC	434795	25.00	ppb	0.16
3) Chlorobenzene-D5 (IS)	11.75	TIC	1069734m	25.00	ppb	0.00
4) 1,4-Dichlorobenzene (IS)	10.94	TIC	7262m	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds Qvalue

Data File : M:\MAX\DATA\211111\1115M14.D  
 Acq On : 15 Nov 21 14:40  
 Sample : BA46116W01  
 Misc : IS&S 8/4/21

Vial: 14  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 22 16:26 2021

Quant Results File: M0825SUR.RE

Quant Method : M:\MAX\DATA\210922\M0825SUR.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Thu Aug 26 11:16:48 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.38	96	356047	25.00	ppb	0.16
4) Chlorobenzene-D5 (IS)	9.53	117	341407	25.00	ppb	0.12
7) 1,4-Dichlorobenzene-D (IS)	11.85	152	199848	25.00	ppb	0.11
<b>System Monitoring Compounds</b>						
2) Dibromofluoromethane(S)	5.60	111	125188	29.15	ppb	0.18
Spiked Amount	25.000		Recovery	=	116.620%	
3) 1,2-DCA-D4(S)	5.98	65	84968	30.11	ppb	0.17
Spiked Amount	25.000		Recovery	=	120.444%	
5) Toluene-D8(S)	8.08	98	382728	23.91	ppb	0.13
Spiked Amount	25.000		Recovery	=	95.624%	
6) 4-Bromofluorobenzene(S)	10.71	95	147342	23.59	ppb	0.11
Spiked Amount	25.000		Recovery	=	94.356%	

Target Compounds

Qvalue

Quantitation Report


Data File : M:\MAX\DATA\211111\1115M14.D  
Acq On : 15 Nov 21 14:40  
Sample : BA46116W01  
Misc : IS&S 8/4/21

Vial: 14  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Nov 22 16:13 2021

Quant Results File: MGAS0825.RE

Method : M:\MAX\DATA\210922\MGAS0825.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Aug 26 16:19:36 2021  
Response via : Initial Calibration





Data File : M:\MAX\DATA\211111\1115M08.D  
Acq On : 15 Nov 21 11:50  
Sample : 211115A BLK  
Misc : IS&S 8/4/21

Vial: 8  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Nov 22 16:12 2021

Quant Results File: MGAS0825.RES

Quant Method : M:\MAX\DATA\210922\MGAS0825.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Aug 26 16:19:36 2021  
Response via : Initial Calibration  
DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.38	TIC	452871	25.00	ppb	0.17
3) Chlorobenzene-D5 (IS)	11.75	TIC	1100001m	25.00	ppb	0.00
4) 1,4-Dichlorobenzene (IS)	10.94	TIC	11606m	25.00	ppb	0.00

#### System Monitoring Compounds

Target Compounds

Qvalue

Data File : M:\MAX\DATA\211111\1115M08.D  
 Acq On : 15 Nov 21 11:50  
 Sample : 211115A BLK  
 Misc : IS&S 8/4/21

Vial: 8  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 22 16:26 2021

Quant Results File: M0825SUR.RES

Quant Method : M:\MAX\DATA\210922\M0825SUR.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Thu Aug 26 11:16:48 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.38	96	371382	25.00	ppb	0.17
4) Chlorobenzene-D5 (IS)	9.53	117	350184	25.00	ppb	0.12
7) 1,4-Dichlorobenzene-D (IS)	11.85	152	211146	25.00	ppb	0.11
System Monitoring Compounds						
2) Dibromofluoromethane(S)	5.60	111	126243	28.19	ppb	0.18
Spiked Amount	25.000		Recovery	=	112.748%	
3) 1,2-DCA-D4(S)	5.98	65	84272	28.63	ppb	0.17
Spiked Amount	25.000		Recovery	=	114.528%	
5) Toluene-D8(S)	8.08	98	406449	24.75	ppb	0.13
Spiked Amount	25.000		Recovery	=	99.004%	
6) 4-Bromofluorobenzene(S)	10.71	95	157554	24.59	ppb	0.11
Spiked Amount	25.000		Recovery	=	98.368%	

Target Compounds

Qvalue

Quantitation Report


Data File : M:\MAX\DATA\211111\1115M08.D  
Acq On : 15 Nov 21 11:50  
Sample : 211115A BLK  
Misc : IS&S 8/4/21

Vial: 8  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Nov 22 16:12 2021

Quant Results File: MGAS0825.RES

Method : M:\MAX\DATA\210922\MGAS0825.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Aug 26 16:19:36 2021  
Response via : Initial Calibration



Data File : M:\THOR\DATA\211111\1119T37.D Vial: 37  
 Acq On : 20 Nov 21 00:39 Operator:  
 Sample : 211119B BLK Inst : Thor  
 Misc : IS&S 8/15/21 Multiplr: 1.00

Quant Time: Nov 22 12:49 2021 Quant Results File: TGAS1015.RES

Quant Method : M:\THOR\DATA\211015\TGAS1015.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Thu Oct 21 10:04:41 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.35	TIC	253167	25.00	ppb	0.00
3) Chlorobenzene-D5 (IS)	12.37	TIC	481529	25.00	ppb	0.00
4) 1,4-Dichlorobenzene-D (IS)	12.37	TIC	481529	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds Qvalue

Data File : M:\THOR\DATA\211111\1119T37.D Vial: 37  
 Acq On : 20 Nov 21 00:39 Operator:  
 Sample : 211119B BLK Inst : Thor  
 Misc : IS&S 8/15/21 Multiplr: 1.00

Quant Time: Nov 22 12:51 2021

Quant Results File: TSUR05.RES

Quant Method : M:\THOR\DATA\211015\TSUR05.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Sun Oct 24 10:14:29 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.35	96	253531	25.00	ppb	0.00
5) Chlorobenzene-D5 (IS)	9.81	117	256331	25.00	ppb	0.00
8) 1,4-Dichlorobenzene-D (IS)	12.37	152	187736	25.00	ppb	0.00
System Monitoring Compounds						
2) Dibromofluoromethane(S)	5.50	111	80071	31.66	ppb	0.00
Spiked Amount	25.000		Recovery	=	126.632%	
3) 1,2-DCA-D4(S)	5.91	65	88306	31.84	ppb	0.00
Spiked Amount	25.000		Recovery	=	127.368%	
6) Toluene-D8(S)	8.22	98	260114	24.47	ppb	0.00
Spiked Amount	25.000		Recovery	=	97.900%	
7) 4-Bromofluorobenzene(S)	11.11	95	102793	25.63	ppb	0.00
Spiked Amount	25.000		Recovery	=	102.504%	

Target Compounds

Qvalue

Quantitation Report


Data File : M:\THOR\DATA\211111\1119T37.D  
Acq On : 20 Nov 21 00:39  
Sample : 211119B BLK  
Misc : IS&S 8/15/21

Vial: 37  
Operator:  
Inst : Thor  
Multiplr: 1.00

Quant Time: Nov 22 12:49 2021

Quant Results File: TGAS1015.RES

Method : M:\THOR\DATA\211015\TGAS1015.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Oct 21 10:04:41 2021  
Response via : Initial Calibration



Data File : M:\MAX\DATA\211111\1115M06.D  
 Acq On : 15 Nov 21 10:53  
 Sample : 211115A LCS 300ug/L  
 Misc : IS&S 8/4/21

Vial: 6  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 15 11:28 2021

Quant Results File: MGAS0825.RES

Quant Method : M:\MAX\DATA\210922\MGAS0825.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Thu Aug 26 16:19:36 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.38	TIC	457583	25.00	ppb	0.17
3) Chlorobenzene-D5 (IS)	11.75	TIC	1146086m	25.00	ppb	0.00
4) 1,4-Dichlorobenzene (IS)	10.94	TIC	133974m	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Gasoline C6-C10	8.08	TIC	7136370m	327.03	ppb	100

Data File : M:\MAX\DATA\211111\1115M06.D Vial: 6  
 Acq On : 15 Nov 21 10:53 Operator: LP,DG,CH  
 Sample : 211115A LCS 300ug/L Inst : Max  
 Misc : IS&S 8/4/21 Multiplr: 1.00

Quant Time: Nov 22 16:29 2021

Quant Results File: M0825SUR.RES

Quant Method : M:\MAX\DATA\210922\M0825SUR.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Thu Aug 26 11:16:48 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.38	96	370711	25.00	ppb	0.17
4) Chlorobenzene-D5 (IS)	9.53	117	351312	25.00	ppb	0.12
7) 1,4-Dichlorobenzene-D (IS)	11.85	152	220509	25.00	ppb	0.11
System Monitoring Compounds						
2) Dibromofluoromethane(S)	5.60	111	125336	28.03	ppb	0.18
Spiked Amount	25.000		Recovery	=	112.140%	
3) 1,2-DCA-D4(S)	5.99	65	86288	29.37	ppb	0.17
Spiked Amount	25.000		Recovery	=	117.480%	
5) Toluene-D8(S)	8.08	98	411713	24.99	ppb	0.13
Spiked Amount	25.000		Recovery	=	99.964%	
6) 4-Bromofluorobenzene(S)	10.71	95	157564	24.51	ppb	0.11
Spiked Amount	25.000		Recovery	=	98.056%	

Target Compounds Qvalue



Quantitation Report


Data File : M:\MAX\DATA\211111\1115M06.D  
Acq On : 15 Nov 21 10:53  
Sample : 211115A LCS 300ug/L  
Misc : IS&S 8/4/21

Vial: 6  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Nov 15 11:28 2021

Quant Results File: MGAS0825.RES

Method : M:\MAX\DATA\210922\MGAS0825.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Aug 26 16:19:36 2021  
Response via : Initial Calibration



Data File : M:\THOR\DATA\211111\1119T35.D  
Acq On : 19 Nov 21 23:49  
Sample : 211119B LCS 300ug/L  
Misc : IS&S 8/15/21

Vial: 35  
Operator:  
Inst : Thor  
Multiplr: 1.00

Quant Time: Nov 22 12:43 2021

Quant Results File: TGAS1015.RES

Quant Method : M:\THOR\DATA\211015\TGAS1015.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Oct 21 10:04:41 2021  
Response via : Initial Calibration  
DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.35	TIC	249108	25.00	ppb	0.00
3) Chlorobenzene-D5 (IS)	12.37	TIC	494630	25.00	ppb	0.00
4) 1,4-Dichlorobenzene-D (IS)	12.37	TIC	494630	25.00	ppb	0.00

#### System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Gasoline C6-C10	11.11	TIC	3880518m	302.04	ppb	100

Data File : M:\THOR\DATA\211111\1119T35.D  
 Acq On : 19 Nov 21 23:49  
 Sample : 211119B LCS 300ug/L  
 Misc : IS&S 8/15/21

Vial: 35  
 Operator:  
 Inst : Thor  
 Multiplr: 1.00

Quant Time: Nov 22 12:51 2021

Quant Results File: TSUR05.RES

Quant Method : M:\THOR\DATA\211015\TSUR05.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Sun Oct 24 10:14:29 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.35	96	254603	25.00	ppb	0.00
5) Chlorobenzene-D5 (IS)	9.81	117	262054	25.00	ppb	0.00
8) 1,4-Dichlorobenzene-D (IS)	12.37	152	191660	25.00	ppb	0.00

#### System Monitoring Compounds

2) Dibromofluoromethane(S)	5.49	111	81326	32.02	ppb	0.00
Spiked Amount			25.000	Recovery =		128.076%
3) 1,2-DCA-D4(S)	5.91	65	87619	31.46	ppb	0.00
Spiked Amount			25.000	Recovery =		125.844%
6) Toluene-D8(S)	8.22	98	260999	24.02	ppb	0.00
Spiked Amount			25.000	Recovery =		96.084%
7) 4-Bromofluorobenzene(S)	11.11	95	106791	26.04	ppb	0.00
Spiked Amount			25.000	Recovery =		104.164%

#### Target Compounds

Qvalue

Quantitation Report


Data File : M:\THOR\DATA\211111\1119T35.D  
Acq On : 19 Nov 21 23:49  
Sample : 211119B LCS 300ug/L  
Misc : IS&S 8/15/21

Vial: 35  
Operator:  
Inst : Thor  
Multiplr: 1.00

Quant Time: Nov 22 12:43 2021

Quant Results File: TGAS1015.RES

Method : M:\THOR\DATA\211015\TGAS1015.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Oct 21 10:04:41 2021  
Response via : Initial Calibration



Data File : M:\MAX\DATA\211111\1115M07.D  
 Acq On : 15 Nov 21 11:22  
 Sample : 211115A LCSD 300ug/L  
 Misc : IS&S 8/4/21

Vial: 7  
 Operator: LP,DG,CH  
 Inst : Max  
 Multiplr: 1.00

Quant Time: Nov 22 16:32 2021

Quant Results File: MGAS0825.RES

Quant Method : M:\MAX\DATA\210922\MGAS0825.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Thu Aug 26 16:19:36 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Fluorobenzene (IS)	6.38	TIC	445352	25.00	ppb	0.17
3) Chlorobenzene-D5 (IS)	11.75	TIC	1117845m	25.00	ppb	0.00
4) 1,4-Dichlorobenzene (IS)	10.94	TIC	111978m	25.00	ppb	0.00

System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Gasoline C6-C10	8.08	TIC	6976942m	331.76	ppb	100

Data File : M:\MAX\DATA\211111\1115M07.D Vial: 7  
 Acq On : 15 Nov 21 11:22 Operator: LP,DG,CH  
 Sample : 211115A LCSD 300ug/L Inst : Max  
 Misc : IS&S 8/4/21 Multiplr: 1.00

Quant Time: Nov 22 16:29 2021 Quant Results File: M0825SUR.RES

Quant Method : M:\MAX\DATA\210922\M0825SUR.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Thu Aug 26 11:16:48 2021  
 Response via : Initial Calibration  
 DataAcq Meth : M8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.38	96	360359	25.00	ppb	0.17
4) Chlorobenzene-D5 (IS)	9.53	117	345933	25.00	ppb	0.12
7) 1,4-Dichlorobenzene-D (IS)	11.85	152	216380	25.00	ppb	0.11
System Monitoring Compounds						
2) Dibromofluoromethane (S)	5.60	111	127949	29.44	ppb	0.18
Spiked Amount	25.000		Recovery	= 117.764%		
3) 1,2-DCA-D4 (S)	5.99	65	85992	30.11	ppb	0.17
Spiked Amount	25.000		Recovery	= 120.440%		
5) Toluene-D8 (S)	8.08	98	407167	25.10	ppb	0.13
Spiked Amount	25.000		Recovery	= 100.400%		
6) 4-Bromofluorobenzene (S)	10.71	95	154182	24.36	ppb	0.11
Spiked Amount	25.000		Recovery	= 97.444%		

Target Compounds Qvalue

Quantitation Report


Data File : M:\MAX\DATA\211111\1115M07.D  
Acq On : 15 Nov 21 11:22  
Sample : 211115A LCSD 300ug/L  
Misc : IS&S 8/4/21

Vial: 7  
Operator: LP,DG,CH  
Inst : Max  
Multiplr: 1.00

Quant Time: Nov 22 16:32 2021

Quant Results File: MGAS0825.RES

Method : M:\MAX\DATA\210922\MGAS0825.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Aug 26 16:19:36 2021  
Response via : Initial Calibration



Data File : M:\THOR\DATA\211111\1119T36.D Vial: 36  
 Acq On : 20 Nov 21 00:14 Operator:  
 Sample : 211119B LCSD 300ug/L Inst : Thor  
 Misc : IS&S 8/15/21 Multiplr: 1.00

Quant Time: Nov 22 12:44 2021

Quant Results File: TGAS1015.RES

Quant Method : M:\THOR\DATA\211015\TGAS1015.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Thu Oct 21 10:04:41 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.34	TIC	258950	25.00	ppb	0.00
3) Chlorobenzene-D5 (IS)	12.37	TIC	485199	25.00	ppb	0.00
4) 1,4-Dichlorobenzene-D (IS)	12.37	TIC	485199	25.00	ppb	0.00

## System Monitoring Compounds

Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
2) Gasoline C6-C10	11.11	TIC	4055943m	305.95	ppb	100



Data File : M:\THOR\DATA\211111\1119T36.D Vial: 36  
 Acq On : 20 Nov 21 00:14 Operator:  
 Sample : 211119B LCSD 300ug/L Inst : Thor  
 Misc : IS&S 8/15/21 Multiplr: 1.00

Quant Time: Nov 22 12:51 2021 Quant Results File: TSUR05.RES

Quant Method : M:\THOR\DATA\211015\TSUR05.M (RTE Integrator)  
 Title : METHOD 8260B  
 Last Update : Sun Oct 24 10:14:29 2021  
 Response via : Initial Calibration  
 DataAcq Meth : T8260

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) Fluorobenzene (IS)	6.34	96	259859	25.00	ppb	0.00
5) Chlorobenzene-D5 (IS)	9.81	117	258203	25.00	ppb	0.00
8) 1,4-Dichlorobenzene-D (IS)	12.37	152	191706	25.00	ppb	0.00
System Monitoring Compounds						
2) Dibromofluoromethane(S)	5.49	111	82978	32.01	ppb	0.00
Spiked Amount	25.000		Recovery	= 128.036%		
3) 1,2-DCA-D4(S)	5.91	65	88746	31.22	ppb	0.00
Spiked Amount	25.000		Recovery	= 124.884%		
6) Toluene-D8(S)	8.22	98	263657	24.63	ppb	0.00
Spiked Amount	25.000		Recovery	= 98.512%		
7) 4-Bromofluorobenzene(S)	11.11	95	106891	26.45	ppb	0.00
Spiked Amount	25.000		Recovery	= 105.816%		

Target Compounds Qvalue

Quantitation Report


Data File : M:\THOR\DATA\211111\1119T36.D  
Acq On : 20 Nov 21 00:14  
Sample : 211119B LCSD 300ug/L  
Misc : IS&S 8/15/21

Vial: 36  
Operator:  
Inst : Thor  
Multiplr: 1.00

Quant Time: Nov 22 12:44 2021

Quant Results File: TGAS1015.RES

Method : M:\THOR\DATA\211015\TGAS1015.M (RTE Integrator)  
Title : METHOD 8260B  
Last Update : Thu Oct 21 10:04:41 2021  
Response via : Initial Calibration



### MAX 8260 Standard Prep

MAX 8260 Water Calibration Curve										
0.3ug/L						Prepared By (Initials): CH				
Prepared: 8/25/2021										
Expires: 9/8/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 9	Various	0.3ug/L	5	Prepared 08/24/21	10/23/2021	N/A	3uL	50mL	P&T Water	0.3
VOA STD. 1	Absolute		50	Prepared 08/24/21	10/23/2021	N/A	5uL			5
VOA STD. 2	Phenova		100	Prepared 08/24/21	10/23/2021	N/A	2.5uL			5
VOA STD. TBA	Various		250	Prepared 08/24/21	9/8/2021	N/A	2uL			10
0.5ug/L										
Prepared: 8/25/2021										
Expires: 9/8/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 9	Various	0.5ug/L	5	Prepared 08/24/21	10/23/2021	N/A	5uL	50mL	P&T Water	0.5
VOA STD. 1	Absolute		50	Prepared 08/24/21	10/23/2021	N/A	10uL			10
VOA STD. 2	Phenova		100	Prepared 08/24/21	10/23/2021	N/A	5uL			10
VOA STD. TBA	Various		250	Prepared 08/24/21	9/8/2021	N/A	5uL			25
1.0ug/L										
Prepared: 8/25/2021										
Expires: 9/8/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 9	Various	1.0ug/L	5	Prepared 08/24/21	10/23/2021	N/A	10uL	50mL	P&T Water	1
VOA STD. 1	Absolute		50	Prepared 08/24/21	10/23/2021	N/A	20uL			20
VOA STD. 2	Phenova		100	Prepared 08/24/21	10/23/2021	N/A	10uL			20
VOA STD. TBA	Various		250	Prepared 08/24/21	9/8/2021	N/A	10uL			50
2.0ug/L										
Prepared: 8/25/2021										
Expires: 9/8/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 9	Various	2.0ug/L	5	Prepared 08/24/21	10/23/2021	N/A	20uL	50mL	P&T Water	2
VOA STD. 1	Absolute		50	Prepared 08/24/21	10/23/2021	N/A	30uL			30
VOA STD. 2	Phenova		100	Prepared 08/24/21	10/23/2021	N/A	15uL			30
VOA STD. TBA	Various		250	Prepared 08/24/21	9/8/2021	N/A	15uL			75
5ug/L										
Prepared: 8/25/2021										
Expires: 9/8/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	5ug/L	50	Prepared 08/24/21	10/23/2021	N/A	5uL	50mL	P&T Water	5
VOA STD. 8	Phenova		50	Prepared 08/24/21	9/8/2021	N/A	5uL			5
VOA STD. 1	Absolute		50	Prepared 08/24/21	10/23/2021	N/A	40uL			40
VOA STD. 2	Phenova		100	Prepared 08/24/21	10/23/2021	N/A	20uL			20
VOA STD. TBA	Various		250	Prepared 08/24/21	9/8/2021	N/A	20uL			100
10ug/L										
Prepared: 8/25/2021										
Expires: 9/8/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	10ug/L	50	Prepared 08/24/21	10/23/2021	N/A	10uL	50mL	P&T Water	10
VOA STD. 8	Phenova		50	Prepared 08/24/21	9/8/2021	N/A	10uL			10
VOA STD. 1	Absolute		50	Prepared 08/24/21	10/23/2021	N/A	50uL			50
VOA STD. 2	Phenova		100	Prepared 08/24/21	10/23/2021	N/A	25uL			50
VOA STD. TBA	Various		250	Prepared 08/24/21	9/8/2021	N/A	25uL			125

20ug/L										
Prepared: 8/25/2021										
Expires: 9/8/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	20ug/L	50	Prepared 08/24/21	10/23/2021	N/A	20uL	50mL	P&T Water	20
VOA STD. 8	Phenova		50	Prepared 08/24/21	9/8/2021	N/A	20uL			20
VOA STD. 1	Absolute		50	Prepared 08/24/21	10/23/2021	N/A	60uL			60
VOA STD. 2	Phenova		100	Prepared 08/24/21	10/23/2021	N/A	30uL			60
VOA STD. TBA	Various		250	Prepared 08/24/21	9/8/2021	N/A	30uL			150
40ug/L										
Prepared: 8/25/2021										
Expires: 9/8/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	40ug/L	50	Prepared 08/24/21	10/23/2021	N/A	40uL	50mL	P&T Water	40
VOA STD. 8	Phenova		50	Prepared 08/24/21	9/8/2021	N/A	40uL			40
VOA STD. 1	Absolute		50	Prepared 08/24/21	10/23/2021	N/A	80uL			80
VOA STD. 2	Phenova		100	Prepared 08/24/21	10/23/2021	N/A	40uL			80
VOA STD. TBA	Various		250	Prepared 08/24/21	9/8/2021	N/A	35uL			175
100ug/L										
Prepared: 8/25/2021										
Expires: 9/8/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	100ug/L	50	Prepared 08/24/21	10/23/2021	N/A	100uL	50mL	P&T Water	100
VOA STD. 8	Phenova		50	Prepared 08/24/21	9/8/2021	N/A	100uL			100
VOA STD. 1	Absolute		50	Prepared 08/24/21	10/23/2021	N/A	100uL			100
VOA STD. 2	Phenova		100	Prepared 08/24/21	10/23/2021	N/A	50uL			100
VOA STD. TBA	Various		250	Prepared 08/24/21	9/8/2021	N/A	40uL			200
MAX 8260 Water Second Source (SS)										
Prepared: 8/25/2021										
Expires: 9/8/2021										
						Prepared By (Initials): CH				
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 3	Phenova	8260 Water SS	100	Prepared 08/24/21	10/23/2021	N/A	25uL	50mL	P&T Water	50
VOA STD. GASES	Phenova	8260 Water SS	50	Prepared 08/24/21	10/23/2021	N/A	10uL			10
VOA STD. 0	Phenova	8260 Water SS	50	Prepared 08/24/21	10/23/2021	N/A	10uL			10
VOA STD. 2-CEVE	Absolute	8260 Water SS	50	Prepared 08/24/21	8/24/2021	N/A	50uL			50
VOA STD. 6	Various	8260 Water SS	50	Prepared 08/24/21	9/8/2021	N/A	10uL			10
VOA STD. TBA	Various	8260 Water SS	250	Prepared 08/24/21	9/8/2021	N/A	25uL			250
8260 Water Continuing Calibrations (CCV)/ Lab Control Spikes (LCS)										
Prepared: 8/25/2021										
Expires: 8/26/2021										
						Prepared By (Initials): CH				
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	CCV/ LCS	50	Prepared 08/24/21	10/23/2021	N/A	10uL	50mL	P&T Water	10
VOA STD. 8	Phenova	CCV/ LCS	50	Prepared 08/24/21	9/8/2021	N/A	10uL			10
VOA STD. 1	Absolute	CCV/ LCS	50	Prepared 08/24/21	10/23/2021	N/A	50uL			50
VOA STD. 2	Phenova	CCV/ LCS	100	Prepared 08/24/21	10/23/2021	N/A	25uL			50
VOA STD. TBA	Various	CCV/ LCS	250	Prepared 08/24/21	9/8/2021	N/A	25uL			250

### THOR 8260 Standard Prep

THOR 8260 Water Calibration Curve										
0.3ug/L						Prepared By (Initials): CH				
Prepared: 10/15/2021										
Expires: 11/3/2021										
Initial Standard Information							Final Standard Information			
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 9	Various	0.3ug/L	5	Prepared 10/13/21	12/12/2021	N/A	3uL	50mL	P&T Water	0.3
VOA STD. 1	Absolute		50	Prepared 10/13/21	12/12/2021	N/A	5uL			5
VOA STD. 2	Phenova		100	Prepared 10/13/21	12/12/2021	N/A	2.5uL			5
VOA STD. TBA	Various		250	Prepared 10/13/21	11/3/2021	N/A	2uL			10
0.5ug/L										
Prepared: 10/15/2021										
Expires: 11/3/2021										
Initial Standard Information							Final Standard Information			
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 9	Various	0.5ug/L	5	Prepared 10/13/21	12/12/2021	N/A	5uL	50mL	P&T Water	0.5
VOA STD. 1	Absolute		50	Prepared 10/13/21	12/12/2021	N/A	10uL			10
VOA STD. 2	Phenova		100	Prepared 10/13/21	12/12/2021	N/A	5uL			10
VOA STD. TBA	Various		250	Prepared 10/13/21	11/3/2021	N/A	5uL			25
1.0ug/L										
Prepared: 10/15/2021										
Expires: 11/3/2021										
Initial Standard Information							Final Standard Information			
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 9	Various	1.0ug/L	5	Prepared 10/13/21	12/12/2021	N/A	10uL	50mL	P&T Water	1
VOA STD. 1	Absolute		50	Prepared 10/13/21	12/12/2021	N/A	20uL			20
VOA STD. 2	Phenova		100	Prepared 10/13/21	12/12/2021	N/A	10uL			20
VOA STD. TBA	Various		250	Prepared 10/13/21	11/3/2021	N/A	10uL			50
2.0ug/L										
Prepared: 10/15/2021										
Expires: 11/3/2021										
Initial Standard Information							Final Standard Information			
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 9	Various	2.0ug/L	5	Prepared 10/13/21	12/12/2021	N/A	20uL	50mL	P&T Water	2
VOA STD. 1	Absolute		50	Prepared 10/13/21	12/12/2021	N/A	30uL			30
VOA STD. 2	Phenova		100	Prepared 10/13/21	12/12/2021	N/A	15uL			30
VOA STD. TBA	Various		250	Prepared 10/13/21	11/3/2021	N/A	15uL			75
5ug/L										
Prepared: 10/15/2021										
Expires: 11/3/2021										
Initial Standard Information							Final Standard Information			
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	5ug/L	50	Prepared 10/13/21	12/12/2021	N/A	5uL	50mL	P&T Water	5
VOA STD. 8	Phenova		50	Prepared 10/13/21	11/3/2021	N/A	5uL			5
VOA STD. 1	Absolute		50	Prepared 10/13/21	12/12/2021	N/A	40uL			40
VOA STD. 2	Phenova		100	Prepared 10/13/21	12/12/2021	N/A	20uL			20
VOA STD. TBA	Various	250	Prepared 10/13/21	11/3/2021	N/A	20uL	100			
10ug/L										
Prepared: 10/15/2021										
Expires: 11/3/2021										
Initial Standard Information							Final Standard Information			
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	10ug/L	50	Prepared 10/13/21	12/12/2021	N/A	10uL	50mL	P&T Water	10
VOA STD. 8	Phenova		50	Prepared 10/13/21	11/3/2021	N/A	10uL			10
VOA STD. 1	Absolute		50	Prepared 10/13/21	12/12/2021	N/A	50uL			50
VOA STD. 2	Phenova		100	Prepared 10/13/21	12/12/2021	N/A	25uL			50
VOA STD. TBA	Various		250	Prepared 10/13/21	11/3/2021	N/A	25uL			125

20ug/L										
Prepared: 10/15/2021										
Expires: 11/3/2021										
Initial Standard Information							Final Standard Information			
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	20ug/L	50	Prepared 10/13/21	12/12/2021	N/A	20uL	50mL	P&T Water	20
VOA STD. 8	Phenova		50	Prepared 10/13/21	11/3/2021	N/A	20uL			20
VOA STD. 1	Absolute		50	Prepared 10/13/21	12/12/2021	N/A	60uL			60
VOA STD. 2	Phenova		100	Prepared 10/13/21	12/12/2021	N/A	30uL			60
VOA STD. TBA	Various		250	Prepared 10/13/21	11/3/2021	N/A	30uL			150
40ug/L										
Prepared: 10/15/2021										
Expires: 11/3/2021										
Initial Standard Information							Final Standard Information			
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	40ug/L	50	Prepared 10/13/21	12/12/2021	N/A	40uL	50mL	P&T Water	40
VOA STD. 8	Phenova		50	Prepared 10/13/21	11/3/2021	N/A	40uL			40
VOA STD. 1	Absolute		50	Prepared 10/13/21	12/12/2021	N/A	80uL			80
VOA STD. 2	Phenova		100	Prepared 10/13/21	12/12/2021	N/A	40uL			80
VOA STD. TBA	Various		250	Prepared 10/13/21	11/3/2021	N/A	35uL			175
100ug/L										
Prepared: 10/15/2021										
Expires: 11/3/2021										
Initial Standard Information							Final Standard Information			
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	100ug/L	50	Prepared 10/13/21	12/12/2021	N/A	100uL	50mL	P&T Water	100
VOA STD. 8	Phenova		50	Prepared 10/13/21	11/3/2021	N/A	100uL			100
VOA STD. 1	Absolute		50	Prepared 10/13/21	12/12/2021	N/A	100uL			100
VOA STD. 2	Phenova		100	Prepared 10/13/21	12/12/2021	N/A	50uL			100
VOA STD. TBA	Various		250	Prepared 10/13/21	11/3/2021	N/A	40uL			200
THOR 8260 Water Second Source (SS)										
Prepared: 10/15/2021										
Expires: 11/3/2021										
Initial Standard Information							Final Standard Information			
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 3	Phenova	8260 Water SS	100	Prepared 10/13/21	12/12/2021	N/A	25uL	50mL	P&T Water	50
VOA STD. GASES	Phenova		50	Prepared 10/13/21	12/12/2021	N/A	10uL			10
VOA STD. 0	Phenova		50	Prepared 10/13/21	12/12/2021	N/A	10uL			10
VOA STD. 2-CEVE	Absolute		50	Prepared 10/13/21	10/13/2021	N/A	50uL			50
VOA STD. 6	Various		50	Prepared 10/13/21	11/3/2021	N/A	10uL			10
VOA STD. TBA	Various		250	Prepared 10/13/21	11/3/2021	N/A	25uL			250
8260 Water Continuing Calibrations (CCV)/ Lab Control Spikes (LCS)										
Prepared: 10/15/2021										
Expires: 10/16/2021										
Initial Standard Information							Final Standard Information			
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA STD. 7	Various	CCV/ LCS	50	Prepared 10/13/21	12/12/2021	N/A	10uL	50mL	P&T Water	10
VOA STD. 8	Phenova		50	Prepared 10/13/21	11/3/2021	N/A	10uL			10
VOA STD. 1	Absolute		50	Prepared 10/13/21	12/12/2021	N/A	50uL			50
VOA STD. 2	Phenova		100	Prepared 10/13/21	12/12/2021	N/A	25uL			50
VOA STD. TBA	Various		250	Prepared 10/13/21	11/3/2021	N/A	25uL			250

### MAX Gas Standard Prep

Gas Primary Working Standard										
Prepared: 6/23/2021						Prepared By (Initials): CH				
Expires: 1/4/2022										
Methanol Lot No.										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	Supplier P/N#	Conc. (ug/mL)	Lot Number - QA Number	Exp. Date (1 yr)	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/mL)
50,000ug/mL Gas STD	Restek	30205	50,000	A0132443	1/4/2022	12/31/2024	80uL	2mL	Methanol	2,000
Gas Second Source (SS) Working Standard										
Prepared: 3/31/2021						Prepared By (Initials): CH				
Expires: 1/31/1930										
Methanol Lot No.										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	Supplier P/N#	Conc. (ug/mL)	Lot Number - QA Number	Exp. Date (1 yr)	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/mL)
Gasoline (50,000ppm)	Phenova	ALO-101543	50,000	CL14915-51175	1/4/2022	1/31/1930	80uL	2mL	Methanol	2,000
MAX Gas Calibration Curve										
Prepared: 8/25/2021						Prepared By (Initials): CH				
Expires: 10/24/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
VOA Gasses Standards	Phenova	20ug/L	2,000	Prepared 06/23/21	1/4/2022	N/A	1uL	100mL	P&T Water	20
VOA Gasses Standards	Phenova	50ug/L	2,000	Prepared 06/23/21	1/4/2022	N/A	2.5uL	100mL	P&T Water	50
VOA Gasses Standards	Phenova	100ug/L	2,000	Prepared 06/23/21	1/4/2022	N/A	5uL	100mL	P&T Water	100
VOA Gasses Standards	Phenova	300ug/L	2,000	Prepared 06/23/21	1/4/2022	N/A	15uL	100mL	P&T Water	300
VOA Gasses Standards	Phenova	600ug/L	2,000	Prepared 06/23/21	1/4/2022	N/A	30uL	100mL	P&T Water	600
VOA Gasses Standards	Phenova	800ug/L	2,000	Prepared 06/23/21	1/4/2022	N/A	40uL	100mL	P&T Water	800
VOA Gasses Standards	Phenova	1,000ug/L	2,000	Prepared 06/23/21	1/4/2022	N/A	50uL	100mL	P&T Water	1,000
Zeus Gas Second Source										
Prepared: 8/25/2021						Prepared By (Initials): CH				
Expires: 10/24/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)
50,000ug/mL Gas STD	Phenova	SS 300ug/L	2,000	Prepared 03/31/21	1/31/1930	N/A	15uL	100mL	P&T Water	300
MAX Gas Continuing Calibrations/Lab Control Spikes										
Prepared: 8/25/2021						Prepared By (Initials): CH				
Expires: 8/26/2021										
Initial Standard Information						Final Standard Information				
Name of Initial Standard (QAU Label)	Supplier	Supplier P/N#	Conc. (ug/mL)	Lot Number - QA Number	Exp. Date (1 yr)	Exp. Date (Manufacturers)	Aliquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/mL)
VOA Gasses Standards	Phenova	300ug/L	2,000	Prepared 06/23/21	1/4/2022	N/A	15uL	100mL	P&T Water	300

### THOR Gas Standard Prep

Gas Primary Working Standard											
Prepared: 6/23/2021						Prepared By (Initials): CH					
Expires: 1/4/2022											
Methanol Lot No.											
Initial Standard Information						Final Standard Information					
Name of Initial Standard (QAU Label)	Supplier	Supplier P/N#	Conc. (ug/mL)	Lot Number - QA Number	Exp. Date (1 yr)	Exp. Date (Manufacturers)	Allquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/mL)	
50,000ug/mL Gas STD	Restek	30205	50,000	A0132443	1/4/2022	12/31/2024	80uL	2mL	Methanol	2,000	
Gas Second Source (SS) Working Standard											
Prepared: 3/31/2021						Prepared By (Initials): CH					
Expires: 1/31/1930											
Methanol Lot No.											
Initial Standard Information						Final Standard Information					
Name of Initial Standard (QAU Label)	Supplier	Supplier P/N#	Conc. (ug/mL)	Lot Number - QA Number	Exp. Date (1 yr)	Exp. Date (Manufacturers)	Allquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/mL)	
Gasoline (50,000ppm)	Phenova	ALO-101543	50,000	CL14915-51175	1/4/2022	1/31/1930	80uL	2mL	Methanol	2,000	
THOR Gas Calibration Curve											
Prepared: 10/15/2021						Prepared By (Initials): CH					
Expires: 12/14/2021											
Initial Standard Information						Final Standard Information					
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Allquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)	
VOA Gasses Standards	Phenova	20ug/L	2,000	Prepared 06/23/21	1/4/2022	N/A	1uL	100mL	P&T Water	20	
VOA Gasses Standards	Phenova	50ug/L	2,000	Prepared 06/23/21	1/4/2022	N/A	2.5uL	100mL	P&T Water	50	
VOA Gasses Standards	Phenova	100ug/L	2,000	Prepared 06/23/21	1/4/2022	N/A	5uL	100mL	P&T Water	100	
VOA Gasses Standards	Phenova	300ug/L	2,000	Prepared 06/23/21	1/4/2022	N/A	15uL	100mL	P&T Water	300	
VOA Gasses Standards	Phenova	600ug/L	2,000	Prepared 06/23/21	1/4/2022	N/A	30uL	100mL	P&T Water	600	
VOA Gasses Standards	Phenova	800ug/L	2,000	Prepared 06/23/21	1/4/2022	N/A	40uL	100mL	P&T Water	800	
VOA Gasses Standards	Phenova	1,000ug/L	2,000	Prepared 06/23/21	1/4/2022	N/A	50uL	100mL	P&T Water	1,000	
Zeus Gas Second Source											
Prepared: 10/15/2021						Prepared By (Initials): CH					
Expires: 12/14/2021											
Initial Standard Information						Final Standard Information					
Name of Initial Standard (QAU Label)	Supplier	APPL Mix Name	Conc. (ug/mL)	Reference To APPL Prep Date	Exp. Date	Exp. Date (Manufacturers)	Allquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/L)	
50,000ug/mL Gas STD	Phenova	SS 300ug/L	2,000	Prepared 03/31/21	1/31/1930	N/A	15uL	100mL	P&T Water	300	
THOR Gas Continuing Calibrations/Lab Control Spikes											
Prepared: 10/15/2021						Prepared By (Initials): CH					
Expires: 10/16/2021											
Initial Standard Information						Final Standard Information					
Name of Initial Standard (QAU Label)	Supplier	Supplier P/N#	Conc. (ug/mL)	Lot Number - QA Number	Exp. Date (1 yr)	Exp. Date (Manufacturers)	Allquot From Stock	Final Volume	Solvent	Final Standard Conc. (ug/mL)	
VOA Gasses Standards	Phenova	300ug/L	2,000	Prepared 06/23/21	1/4/2022	N/A	15uL	100mL	P&T Water	300	



# Injection Log

Directory: M:\MAX\DATA\210825\

Line	Vial	FileName	Multiplier	SampleName	Misc Info	Injected
1	2	0825M12.D	1	0.3ug/L VOC STD 8/25/21	IS&S 6/4/21	25 Aug 21 15:15
2	3	0825M13.D	1	0.5ug/L VOC STD 8/25/21	IS&S 6/4/21	25 Aug 21 15:43
3	4	0825M14.D	1	1ug/L VOC STD 8/25/21	IS&S 6/4/21	25 Aug 21 16:11
4	5	0825M15.D	1	2ug/L VOC STD 8/25/21	IS&S 6/4/21	25 Aug 21 16:39
5	6	0825M16.D	1	5ug/L VOC STD 8/25/21	IS&S 6/4/21	25 Aug 21 17:07
6	7	0825M17.D	1	10ug/L VOC STD 8/25/21	IS&S 6/4/21	25 Aug 21 17:35
7	8	0825M18.D	1	20ug/L VOC STD 8/25/21	IS&S 6/4/21	25 Aug 21 18:03
8	9	0825M19.D	1	40ug/L VOC STD 8/25/21	IS&S 6/4/21	25 Aug 21 18:31
9	10	0825M20.D	1	100ug/L VOC STD 8/25/21	IS&S 6/4/21	25 Aug 21 18:59
10	13	0825M23.D	1	20ug/L GAS STD 8/25/21	IS&S 6/4/21	25 Aug 21 20:23
11	14	0825M24.D	1	50ug/L GAS STD 8/25/21	IS&S 6/4/21	25 Aug 21 20:51
12	15	0825M25.D	1	100ug/L GAS STD 8/25/21	IS&S 6/4/21	25 Aug 21 21:19
13	16	0825M26.D	1	300ug/L GAS STD 8/25/21	IS&S 6/4/21	25 Aug 21 21:47
14	17	0825M27.D	1	600ug/L GAS STD 8/25/21	IS&S 6/4/21	25 Aug 21 22:14
15	18	0825M28.D	1	800ug/L GAS STD 8/25/21	IS&S 6/4/21	25 Aug 21 22:42
16	19	0825M29.D	1	1000ug/L GAS STD 8/25/21	IS&S 6/4/21	25 Aug 21 23:10
17	21	0825M31.D	1	(SS) 300ug/L GAS STD 8/25/21	IS&S 6/4/21	26 Aug 21 00:06

# Injection Log

Directory: M:\THOR\DATA\211015\

Line	Vial	FileName	Multiplier	SampleName	Misc Info	Injected
1	8	1015B08.D	1	0.3ug/L VOC STD 10/11/21	IS&S 8/15/21	15 Oct 21 15:28
2	9	1015B09.D	1	0.5ug/L VOC STD 10/11/21	IS&S 8/15/21	15 Oct 21 15:53
3	10	1015B10.D	1	1ug/L VOC STD 10/11/21	IS&S 8/15/21	15 Oct 21 16:18
4	11	1015B11.D	1	2ug/L VOC STD 10/11/21	IS&S 8/15/21	15 Oct 21 16:43
5	12	1015B12.D	1	5ug/L VOC STD 10/11/21	IS&S 8/15/21	15 Oct 21 17:07
6	13	1015B13.D	1	10ug/L VOC STD 10/11/21	IS&S 8/15/21	15 Oct 21 17:32
7	14	1015B14.D	1	20ug/L VOC STD 10/11/21	IS&S 8/15/21	15 Oct 21 17:57
8	15	1015B15.D	1	40ug/L VOC STD 10/11/21	IS&S 8/15/21	15 Oct 21 18:22
9	16	1015B16.D	1	100ug/L VOC STD 10/11/21	IS&S 8/15/21	15 Oct 21 18:47
10	19	1015B19.D	1	20 ug/L GAS STD 10/15/21	IS&S 8/15/21	15 Oct 21 20:01
11	20	1015B20.D	1	50 ug/L GAS STD 10/15/21	IS&S 8/15/21	15 Oct 21 20:26
12	21	1015B21.D	1	100 ug/L GAS STD 10/15/21	IS&S 8/15/21	15 Oct 21 20:51
13	22	1015B22.D	1	300 ug/L GAS STD 10/15/21	IS&S 8/15/21	15 Oct 21 21:16
14	23	1015B23.D	1	600 ug/L GAS STD 10/15/21	IS&S 8/15/21	15 Oct 21 21:40
15	24	1015B24.D	1	800 ug/L GAS STD 10/15/21	IS&S 8/15/21	15 Oct 21 22:05
16	25	1015B25.D	1	1000 ug/L GAS STD 10/15/21	IS&S 8/15/21	15 Oct 21 22:30
17	27	1015B27.D	1	(SS) 300ug/L GAS STD 10/15/21	IS&S 8/15/21	15 Oct 21 23:19

## Injection Log

Directory: M:\MAX\DATA\211111\

Line	Vial	FileName	Multiplier	SampleName	Misc Info	Injected
1	5	1115M05.D	1	211115A CCV 300ug/L	IS&S 8/4/21	15 Nov 21 10:25
2	6	1115M06.D	1	211115A LCS 300ug/L	IS&S 8/4/21	15 Nov 21 10:53
3	7	1115M07.D	1	211115A LCSD 300ug/L	IS&S 8/4/21	15 Nov 21 11:22
4	8	1115M08.D	1	211115A BLK	IS&S 8/4/21	15 Nov 21 11:50
5	12	1115M12.D	1	BA46114W01	IS&S 8/4/21	15 Nov 21 13:44
6	13	1115M13.D	1	BA46115W01	IS&S 8/4/21	15 Nov 21 14:12
7	14	1115M14.D	1	BA46116W01	IS&S 8/4/21	15 Nov 21 14:40
8	26	1115M26.D	1	Ending CCV 300ug/L 11/15/21	IS&S 8/4/21	15 Nov 21 20:21

## Injection Log

Directory: M:\THOR\DATA\211111\

Line	Vial	FileName	Multiplier	SampleName	Misc Info	Injected
1	34	1119T34.D	1	211119B CCV 300ug/L	IS&S 8/15/21	19 Nov 21 23:25
2	35	1119T35.D	1	211119B LCS 300ug/L	IS&S 8/15/21	19 Nov 21 23:49
3	36	1119T36.D	1	211119B LCSD 300ug/L	IS&S 8/15/21	20 Nov 21 00:14
4	37	1119T37.D	1	211119B BLK	IS&S 8/15/21	20 Nov 21 00:39
5	38	1119T38.D	1	BA46117W07	IS&S 8/15/21	20 Nov 21 1:03
6	53	1119T53.D	1	Ending CCV 300ug/L 11/19/21	IS&S 8/15/21	20 Nov 21 7:11

**INORGANIC ANALYSIS**  
**Calibration and Raw Data**



Name of Final Standard **TOC Calibration Curve**  
 Prep Date 10/25/2021  
 Exp Date 10/25/2022

Prep'd By (Initials) KS

Initial Standard Information						Final Standard Information			
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc.(range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
Total Organic Carbon (TOC) Standard Cal 1	Agilent	IQC-106-5	1000 mg/L	0006588597-51848	3/31/2023	20 uL	40 mL	DI Water	0.5 ppm
Total Organic Carbon (TOC) Standard Cal 2	Agilent	IQC-106-5	1000 mg/L	0006588597-51848	3/31/2023	80 uL	40 mL	DI Water	2 ppm
Total Organic Carbon (TOC) Standard Cal 3	Agilent	IQC-106-5	1000 mg/L	0006588597-51848	3/31/2023	200 uL	40 mL	DI Water	5 ppm
Total Organic Carbon (TOC) Standard Cal 4	Agilent	IQC-106-5	1000 mg/L	0006588597-51848	3/31/2023	400 uL	40 mL	DI Water	10 ppm
Total Organic Carbon (TOC) Standard Cal 5	Agilent	IQC-106-5	1000 mg/L	0006588597-51848	3/31/2023	800 uL	40 mL	DI Water	20 ppm

Name of Final Standard **ICV (TOC)**  
 Prep Date 10/25/2021  
 Exp Date 10/25/2022

Prep'd By (Initials) KS

Initial Standard Information						Final Standard Information			
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc.(range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
1000 PPM ICV TOC Intermediate	APPL Inc.	IQC-106-5	1000 mg/L	0006465171-49409	6/30/2021	400 uL	40mL	DI Water	10 ppm

ICV recertified against the non-expired calibration

Name of Final Standard **CCV (TOC)**  
 Prep Date See Data  
 Exp Date 1 year

Prep'd By (Initials) EA

Initial Standard Information						Final Standard Information			
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc.(range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
Total Organic Carbon (TOC) Standard	Agilent	IQC-1 06-5	1000 mg/L	0006588597-51848	3/31/2023	200 uL	40 mL	DI Water	5 ppm

Name of Final Standard **TOC LCS/LCSD**  
 Prep Date See Data  
 Exp Date 1 year

Prep'd By (Initials) EA

Initial Standard Information						Final Standard Information			
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc.(range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
Total Organic Carbon (TOC) Standard	Agilent	IQC-106-5	1000 mg/L	0006588597-51848	3/31/2023	200 uL	40 mL	DI Water	5 ppm

Name of Final Standard **TOC MS/MSD**  
 Prep Date See Data  
 Exp Date 1 year

Prep'd By (Initials) EA

Initial Standard Information						Final Standard Information			
Name of Initial Standard (from container Label)	Supplier	Supplier P/N# (or APPL Mix Name)	Conc.(range)	Lot # with QA # (or reference to APPL prep date)	Exp Date	Aliquot from Stock	Final Volume	Final Solvent + Lot# (or APPL Prep Date)	Final Standard Conc (range)
Total Organic Carbon (TOC) Standard	Agilent	IQC-106-5	1000 mg/L	0006588597-51848	3/31/2023	200 uL	40 mL	sample	5 ppm