

Energy Laboratories Inc

ANALYTICAL RUN Summary

28-Feb-22

Run ID VOA5975C.I_220104A

Run Start Date: 1/4/2022
 Analyst: Melissa Chavez
 Ical:
 Column ID:
 Comments:

| Instrument ID | Description |
|---------------|-------------|
| Bal #22 | Balance |

| Std ID | Std Name | Std Amount | Std Units | Samp Amount | Samp Units | SampType | Expiration Date |
|-----------|---|------------|-----------|-------------|------------|-------------|-----------------|
| VOCF3473 | Calibration Surrogates | | ul | 42 | ml | CAL | 3/14/2022 |
| VOCF3517 | Internal Standard / Surrogates (INT/SURR) | 8.4 | ul | 42 | ml | MBLK, ICV (| 12/31/2022 |
| VOCF3529B | 2nd Source MtBE | 1.05 | ul | 42 | ml | ICV | 1/29/2022 |
| VOCF3546A | Liquids | | ul | 42 | ml | CAL | 1/13/2022 |
| VOCF3549 | 2nd Source Ketones | 1.05 | ul | 42 | ml | ICV | 1/15/2022 |
| VOCF3550 | Ketones | | ul | 42 | ml | CAL | 1/16/2022 |
| VOCF3558B | 2nd Source Liquids | 1.05 | ul | 42 | ml | ICV | 2/27/2022 |
| VOCF3559A | MtBE | | ul | 42 | ml | CAL | 1/27/2022 |
| VOCF3562A | Gases | | ul | 42 | ml | CAL | 1/10/2022 |
| VOCF3563 | Internals | 8.4 | ul | 42 | ml | CAL | 7/3/2022 |
| VOCF3566A | 2nd Source Gases | 1.05 | ul | 42 | ml | ICV | 1/11/2022 |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|--------------------|--------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|-------|------|---|
| 14970784 | 04JAN08_D_TU | VOC-8260-BFB | TUNE | DA5975C\VG010: | 1/4/2022 2:38:00 | 1 | R372940 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 173, % of mass 174 | A | % | 0 | 0 | | 100 | 0 | 0 | 0 | 0 | 0 | 0% | 0 | 1.99 | 0% | |
| 174, % of mass 95 | A | % | 95.2 | 95.2 | | 100 | 0 | 0 | 0 | 0 | 0 | 95% | 50 | 99.99 | 0% | |
| 175, % of mass 174 | A | % | 6.6 | 6.6 | | 100 | 0 | 0 | 0 | 0 | 0 | 7% | 5 | 9 | 0% | |
| 176, % of mass 174 | A | % | 95.7 | 95.7 | | 100 | 0 | 0 | 0 | 0 | 0 | 96% | 95 | 101 | 0% | |
| 177, % of mass 176 | A | % | 6.7 | 6.7 | | 100 | 0 | 0 | 0 | 0 | 0 | 7% | 5 | 9 | 0% | |
| 50, % of mass 95 | A | % | 21.2 | 21.2 | | 100 | 0 | 0 | 0 | 0 | 0 | 21% | 15 | 40 | 0% | |
| 75, % of mass 95 | A | % | 51 | 51 | | 100 | 0 | 0 | 0 | 0 | 0 | 51% | 30 | 60 | 0% | |
| 95, Base Peak | A | % | 100 | 100 | | 100 | 0 | 0 | 0 | 0 | 0 | 100% | 0 | 100 | 0% | |
| 96, % of mass 95 | A | % | 5.4 | 5.4 | | 100 | 0 | 0 | 0 | 0 | 0 | 5% | 5 | 9 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|-------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970898 | MBLK010422_ | VOC-8260-W-Q | MBLK | DA5975CVVG010 | 1/4/2022 3:05:37 | 1 | R372940 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 1,1,1-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.131 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 1,1,2,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0872 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 1,1,2-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 1,1-Dichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.135 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 1,1-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 1,1-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.083 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 1,2,3-Trichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.235 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 1,2-Dibromoethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0916 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 1,2-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0746 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 1,2-Dichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.116 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 1,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0847 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 1,3-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0803 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 1,3-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0791 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 1,4-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0858 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 2,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.186 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 2-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0876 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 4-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0728 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Benzene | A | ug/L | 0.12327 | 0 | | 0 | 0 | 0 | 0.0914 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Bromobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0831 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Bromochloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Bromodichloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.12 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Bromoform | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.119 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Bromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.253 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Carbon tetrachloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.143 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Chlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0914 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Chlorodibromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0841 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Chloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.169 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Chloroform | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0789 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Chloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.162 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| cis-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| cis-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.073 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Dibromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.147 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Dichlorodifluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.175 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Ethylbenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0836 | 0.5 | 500 | 0% | 0 | 0 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|--------------------------------|-------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970898 | MBLK010422_ | VOC-8260-W-Q | MBLK | DA5975C\VG010 | 1/4/2022 3:05:37 | 1 | R372940 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| m+p-Xylenes | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.15 | 0.5 | 1000 | 0% | 0 | 0 | 0% | |
| Methyl ethyl ketone | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 1.77 | 10 | 5000 | 0% | 0 | 0 | 0% | |
| Methyl tert-butyl ether (MTBE) | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Methylene chloride | A | ug/L | 1.44235 | 0 | | 0 | 0 | 0 | 0.338 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| o-Xylene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0604 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Styrene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.067 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Tetrachloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0671 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Toluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0679 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| trans-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.125 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| trans-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0846 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Trichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0993 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Trichlorofluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.134 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Vinyl chloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.153 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 1,4-Dichlorobenzene-d4 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 0 | 0 | 0% | |
| Chlorobenzene-d5 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 0 | 0 | 0% | |
| Fluorobenzene | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 0 | 0 | 0% | |
| Xylenes, Total | M | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0604 | 0.5 | 1500 | 0% | 0 | 0 | 0% | |
| 1,2-Dichloroethane-d4 | S | ug/L | 279.39635 | 11.175854 | | 10 | 0 | 0 | 0.229 | 0.5 | 500 | 112% | 70 | 130 | 0% | |
| Dibromofluoromethane | S | ug/L | 278.46353 | 11.1385412 | | 10 | 0 | 0 | 0.129 | 0.5 | 500 | 111% | 77 | 126 | 0% | |
| p-Bromofluorobenzene | S | ug/L | 267.28149 | 10.6912596 | | 10 | 0 | 0 | 0.149 | 0.5 | 500 | 107% | 76 | 127 | 0% | |
| Toluene-d8 | S | ug/L | 265.34358 | 10.6137432 | | 10 | 0 | 0 | 0.23 | 0.5 | 500 | 106% | 79 | 122 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970899 | ICAL010422_1 | VOC-8260-W-Q | CAL1 | DA5975C\VG010 | 1/4/2022 3:33:04 | 1 | R372940 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,2-Dichlorobenzene | A | ug/L | 2.73073 | 0.1092292 | | 0.1 | 0 | 0 | 0.0746 | 0.5 | 500 | 109% | 50 | 150 | 0% | |
| 1,2-Dichloroethane | A | ug/L | 2.90899 | 0.1163596 | | 0.1 | 0 | 0 | 0.116 | 0.5 | 500 | 116% | 50 | 150 | 0% | |
| 1,3-Dichlorobenzene | A | ug/L | 2.6327 | 0.105308 | | 0.1 | 0 | 0 | 0.0803 | 0.5 | 500 | 105% | 50 | 150 | 0% | |
| 1,4-Dichlorobenzene | A | ug/L | 2.76134 | 0.1104536 | | 0.1 | 0 | 0 | 0.0858 | 0.5 | 500 | 110% | 50 | 150 | 0% | |
| Benzene | A | ug/L | 2.73933 | 0.1095732 | | 0.1 | 0 | 0 | 0.0914 | 0.5 | 500 | 110% | 50 | 150 | 0% | |
| Chloroform | A | ug/L | 2.89464 | 0.1157856 | | 0.1 | 0 | 0 | 0.0789 | 0.5 | 500 | 116% | 50 | 150 | 0% | |
| Ethylbenzene | A | ug/L | 2.53666 | 0.1014664 | | 0.1 | 0 | 0 | 0.0836 | 0.5 | 500 | 101% | 50 | 150 | 0% | |
| m+p-Xylenes | A | ug/L | 5.07121 | 0.2028484 | | 0.2 | 0 | 0 | 0.15 | 0.5 | 1000 | 101% | 50 | 150 | 0% | |
| Styrene | A | ug/L | 2.16254 | 0.0865016 | | 0.1 | 0 | 0 | 0.067 | 0.5 | 500 | 87% | 50 | 150 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970899 | ICAL010422_1 | VOC-8260-W-Q | CAL1 | DA5975C\VG010 | 1/4/2022 3:33:04 | 1 | R372940 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| Tetrachloroethene | A | ug/L | 2.67723 | 0.1070892 | | 0.1 | 0 | 0 | 0.0671 | 0.5 | 500 | 107% | 50 | 150 | 0% | |
| Toluene | A | ug/L | 2.6145 | 0.10458 | | 0.1 | 0 | 0 | 0.0679 | 0.5 | 500 | 105% | 50 | 150 | 0% | |
| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
| 14970901 | ICAL010422_2 | VOC-8260-W-Q | CAL2 | DA5975C\VG010 | 1/4/2022 4:00:35 | 1 | R372940 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A | ug/L | 12.82253 | 0.5129012 | | 0.5 | 0 | 0 | 0.101 | 0.5 | 500 | 103% | 50 | 150 | 0% | |
| 1,1,1-Trichloroethane | A | ug/L | 12.18907 | 0.4875628 | | 0.5 | 0 | 0 | 0.131 | 0.5 | 500 | 98% | 50 | 150 | 0% | |
| 1,1,2,2-Tetrachloroethane | A | ug/L | 12.84375 | 0.51375 | | 0.5 | 0 | 0 | 0.0872 | 0.5 | 500 | 103% | 50 | 150 | 0% | |
| 1,1,2-Trichloroethane | A | ug/L | 13.23404 | 0.5293616 | | 0.5 | 0 | 0 | 0.108 | 0.5 | 500 | 106% | 50 | 150 | 0% | |
| 1,1-Dichloroethane | A | ug/L | 12.06522 | 0.4826088 | | 0.5 | 0 | 0 | 0.135 | 0.5 | 500 | 97% | 50 | 150 | 0% | |
| 1,1-Dichloroethene | A | ug/L | 11.90807 | 0.4763228 | | 0.5 | 0 | 0 | 0.141 | 0.5 | 500 | 95% | 50 | 150 | 0% | |
| 1,1-Dichloropropene | A | ug/L | 11.33971 | 0.4535884 | | 0.5 | 0 | 0 | 0.083 | 0.5 | 500 | 91% | 50 | 150 | 0% | |
| 1,2,3-Trichloropropane | A | ug/L | 13.70838 | 0.5483352 | | 0.5 | 0 | 0 | 0.235 | 0.5 | 500 | 110% | 50 | 150 | 0% | |
| 1,2-Dibromoethane | A | ug/L | 12.86397 | 0.5145588 | | 0.5 | 0 | 0 | 0.0916 | 0.5 | 500 | 103% | 50 | 150 | 0% | |
| 1,2-Dichlorobenzene | A | ug/L | 12.14234 | 0.4856936 | | 0.5 | 0 | 0 | 0.0746 | 0.5 | 500 | 97% | 70 | 130 | 0% | |
| 1,2-Dichloroethane | A | ug/L | 12.39059 | 0.4956236 | | 0.5 | 0 | 0 | 0.116 | 0.5 | 500 | 99% | 70 | 130 | 0% | |
| 1,2-Dichloropropane | A | ug/L | 12.0602 | 0.482408 | | 0.5 | 0 | 0 | 0.0847 | 0.5 | 500 | 96% | 50 | 150 | 0% | |
| 1,3-Dichlorobenzene | A | ug/L | 11.84726 | 0.4738904 | | 0.5 | 0 | 0 | 0.0803 | 0.5 | 500 | 95% | 70 | 130 | 0% | |
| 1,3-Dichloropropane | A | ug/L | 11.85262 | 0.4741048 | | 0.5 | 0 | 0 | 0.0791 | 0.5 | 500 | 95% | 50 | 150 | 0% | |
| 1,4-Dichlorobenzene | A | ug/L | 11.96618 | 0.4786472 | | 0.5 | 0 | 0 | 0.0858 | 0.5 | 500 | 96% | 70 | 130 | 0% | |
| 2,2-Dichloropropane | A | ug/L | 12.48201 | 0.4992804 | | 0.5 | 0 | 0 | 0.186 | 0.5 | 500 | 100% | 50 | 150 | 0% | |
| 2-Chlorotoluene | A | ug/L | 11.19768 | 0.4479072 | | 0.5 | 0 | 0 | 0.0876 | 0.5 | 500 | 90% | 50 | 150 | 0% | |
| 4-Chlorotoluene | A | ug/L | 11.22327 | 0.4489308 | | 0.5 | 0 | 0 | 0.0728 | 0.5 | 500 | 90% | 50 | 150 | 0% | |
| Benzene | A | ug/L | 12.18007 | 0.4872028 | | 0.5 | 0 | 0 | 0.0914 | 0.5 | 500 | 97% | 70 | 130 | 0% | |
| Bromobenzene | A | ug/L | 12.331 | 0.49324 | | 0.5 | 0 | 0 | 0.0831 | 0.5 | 500 | 99% | 50 | 150 | 0% | |
| Bromochloromethane | A | ug/L | 12.9568 | 0.518272 | | 0.5 | 0 | 0 | 0.141 | 0.5 | 500 | 104% | 50 | 150 | 0% | |
| Bromodichloromethane | A | ug/L | 12.60141 | 0.5040564 | | 0.5 | 0 | 0 | 0.12 | 0.5 | 500 | 101% | 50 | 150 | 0% | |
| Bromoform | A | ug/L | 11.78598 | 0.4714392 | | 0.5 | 0 | 0 | 0.119 | 0.5 | 500 | 94% | 50 | 150 | 0% | |
| Bromomethane | A | ug/L | 12.04638 | 0.4818552 | | 0.5 | 0 | 0 | 0.253 | 0.5 | 500 | 96% | 50 | 150 | 0% | |
| Carbon tetrachloride | A | ug/L | 12.2545 | 0.49018 | | 0.5 | 0 | 0 | 0.143 | 0.5 | 500 | 98% | 50 | 150 | 0% | |
| Chlorobenzene | A | ug/L | 12.52043 | 0.5008172 | | 0.5 | 0 | 0 | 0.0914 | 0.5 | 500 | 100% | 50 | 150 | 0% | |
| Chlorodibromomethane | A | ug/L | 12.83929 | 0.5135716 | | 0.5 | 0 | 0 | 0.0841 | 0.5 | 500 | 103% | 50 | 150 | 0% | |
| Chloroethane | A | ug/L | 14.86697 | 0.5946788 | | 0.5 | 0 | 0 | 0.169 | 0.5 | 500 | 119% | 50 | 150 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|--------------------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970901 | ICAL010422_2 | VOC-8260-W-Q | CAL2 | DA5975C\VG010 | 1/4/2022 4:00:35 | 1 | R372940 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| Chloroform | A | ug/L | 13.06683 | 0.5226732 | | 0.5 | 0 | 0 | 0.0789 | 0.5 | 500 | 105% | 70 | 130 | 0% | |
| Chloromethane | A | ug/L | 13.86612 | 0.5546448 | | 0.5 | 0 | 0 | 0.162 | 0.5 | 500 | 111% | 50 | 150 | 0% | |
| cis-1,2-Dichloroethene | A | ug/L | 12.56593 | 0.5026372 | | 0.5 | 0 | 0 | 0.108 | 0.5 | 500 | 101% | 50 | 150 | 0% | |
| cis-1,3-Dichloropropene | A | ug/L | 12.07376 | 0.4829504 | | 0.5 | 0 | 0 | 0.073 | 0.5 | 500 | 97% | 50 | 150 | 0% | |
| Dibromomethane | A | ug/L | 14.06189 | 0.5624756 | | 0.5 | 0 | 0 | 0.147 | 0.5 | 500 | 112% | 50 | 150 | 0% | |
| Dichlorodifluoromethane | A | ug/L | 12.06625 | 0.48265 | | 0.5 | 0 | 0 | 0.175 | 0.5 | 500 | 97% | 50 | 150 | 0% | |
| Ethylbenzene | A | ug/L | 11.04112 | 0.4416448 | | 0.5 | 0 | 0 | 0.0836 | 0.5 | 500 | 88% | 70 | 130 | 0% | |
| m+p-Xylenes | A | ug/L | 22.14096 | 0.8856384 | | 1 | 0 | 0 | 0.15 | 0.5 | 1000 | 89% | 70 | 130 | 0% | |
| Methyl ethyl ketone | A | ug/L | 122.052 | 4.88208 | | 5 | 0 | 0 | 1.77 | 10 | 5000 | 98% | 50 | 150 | 0% | |
| Methyl tert-butyl ether (MTBE) | A | ug/L | 12.32545 | 0.493018 | | 0.5 | 0 | 0 | 0.101 | 0.5 | 500 | 99% | 50 | 150 | 0% | |
| Methylene chloride | A | ug/L | 15.62358 | 0.6249432 | | 0.5 | 0 | 0 | 0.338 | 0.5 | 500 | 125% | 50 | 150 | 0% | |
| o-Xylene | A | ug/L | 10.66119 | 0.4264476 | | 0.5 | 0 | 0 | 0.0604 | 0.5 | 500 | 85% | 50 | 150 | 0% | |
| Styrene | A | ug/L | 11.49684 | 0.4598736 | | 0.5 | 0 | 0 | 0.067 | 0.5 | 500 | 92% | 70 | 130 | 0% | |
| Tetrachloroethene | A | ug/L | 11.73024 | 0.4692096 | | 0.5 | 0 | 0 | 0.0671 | 0.5 | 500 | 94% | 70 | 130 | 0% | |
| Toluene | A | ug/L | 11.28985 | 0.451594 | | 0.5 | 0 | 0 | 0.0679 | 0.5 | 500 | 90% | 70 | 130 | 0% | |
| trans-1,2-Dichloroethene | A | ug/L | 12.50224 | 0.5000896 | | 0.5 | 0 | 0 | 0.125 | 0.5 | 500 | 100% | 50 | 150 | 0% | |
| trans-1,3-Dichloropropene | A | ug/L | 11.75888 | 0.4703552 | | 0.5 | 0 | 0 | 0.0846 | 0.5 | 500 | 94% | 50 | 150 | 0% | |
| Trichloroethene | A | ug/L | 11.67527 | 0.4670108 | | 0.5 | 0 | 0 | 0.0993 | 0.5 | 500 | 93% | 50 | 150 | 0% | |
| Trichlorofluoromethane | A | ug/L | 11.36372 | 0.4545488 | | 0.5 | 0 | 0 | 0.134 | 0.5 | 500 | 91% | 50 | 150 | 0% | |
| Vinyl chloride | A | ug/L | 12.54456 | 0.5017824 | | 0.5 | 0 | 0 | 0.153 | 0.5 | 500 | 100% | 50 | 150 | 0% | |
| 1,4-Dichlorobenzene-d4 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 50 | 150 | 0% | |
| Chlorobenzene-d5 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 50 | 150 | 0% | |
| Fluorobenzene | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 50 | 150 | 0% | |
| Xylenes, Total | M | ug/L | 32.80215 | 1.312086 | | 1.5 | 0 | 0 | 0.0604 | 0.5 | 1500 | 87% | 50 | 150 | 0% | |
| 1,2-Dichloroethane-d4 | S | ug/L | 12.66005 | 0.506402 | | 0.5 | 0 | 0 | 0.229 | 0.5 | 500 | 101% | 50 | 150 | 0% | |
| Dibromofluoromethane | S | ug/L | 12.59997 | 0.5039988 | | 0.5 | 0 | 0 | 0.129 | 0.5 | 500 | 101% | 50 | 150 | 0% | |
| p-Bromofluorobenzene | S | ug/L | 11.33932 | 0.4535728 | | 0.5 | 0 | 0 | 0.149 | 0.5 | 500 | 91% | 50 | 150 | 0% | |
| Toluene-d8 | S | ug/L | 11.30891 | 0.4523564 | | 0.5 | 0 | 0 | 0.23 | 0.5 | 500 | 90% | 50 | 150 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|----------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970902 | ICAL010422_3 | VOC-8260-W-Q | CAL3 | DA5975C\VG010 | 1/4/2022 4:28:05 | 1 | R372940 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970902 | ICAL010422_3 | VOC-8260-W-Q | CAL3 | DA5975C\VG010 | 1/4/2022 4:28:05 | 1 | R372940 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A | ug/L | 24.15093 | 0.9660372 | | 1 | 0 | 0 | 0.101 | 0.5 | 500 | 97% | 70 | 130 | 0% | |
| 1,1,1-Trichloroethane | A | ug/L | 25.18087 | 1.0072348 | | 1 | 0 | 0 | 0.131 | 0.5 | 500 | 101% | 70 | 130 | 0% | |
| 1,1,2,2-Tetrachloroethane | A | ug/L | 27.78828 | 1.1115312 | | 1 | 0 | 0 | 0.0872 | 0.5 | 500 | 111% | 70 | 130 | 0% | |
| 1,1,2-Trichloroethane | A | ug/L | 25.84 | 1.0336 | | 1 | 0 | 0 | 0.108 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| 1,1-Dichloroethane | A | ug/L | 25.68346 | 1.0273384 | | 1 | 0 | 0 | 0.135 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| 1,1-Dichloroethene | A | ug/L | 25.88489 | 1.0353956 | | 1 | 0 | 0 | 0.141 | 0.5 | 500 | 104% | 70 | 130 | 0% | |
| 1,1-Dichloropropene | A | ug/L | 24.36174 | 0.9744696 | | 1 | 0 | 0 | 0.083 | 0.5 | 500 | 97% | 70 | 130 | 0% | |
| 1,2,3-Trichloropropane | A | ug/L | 26.71444 | 1.0685776 | | 1 | 0 | 0 | 0.235 | 0.5 | 500 | 107% | 70 | 130 | 0% | |
| 1,2-Dibromoethane | A | ug/L | 24.36006 | 0.9744024 | | 1 | 0 | 0 | 0.0916 | 0.5 | 500 | 97% | 70 | 130 | 0% | |
| 1,2-Dichlorobenzene | A | ug/L | 24.94023 | 0.9976092 | | 1 | 0 | 0 | 0.0746 | 0.5 | 500 | 100% | 70 | 130 | 0% | |
| 1,2-Dichloroethane | A | ug/L | 23.46155 | 0.938462 | | 1 | 0 | 0 | 0.116 | 0.5 | 500 | 94% | 70 | 130 | 0% | |
| 1,2-Dichloropropane | A | ug/L | 25.11474 | 1.0045896 | | 1 | 0 | 0 | 0.0847 | 0.5 | 500 | 100% | 70 | 130 | 0% | |
| 1,3-Dichlorobenzene | A | ug/L | 25.77252 | 1.0309008 | | 1 | 0 | 0 | 0.0803 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| 1,3-Dichloropropane | A | ug/L | 24.38386 | 0.9753544 | | 1 | 0 | 0 | 0.0791 | 0.5 | 500 | 98% | 70 | 130 | 0% | |
| 1,4-Dichlorobenzene | A | ug/L | 25.32843 | 1.0131372 | | 1 | 0 | 0 | 0.0858 | 0.5 | 500 | 101% | 70 | 130 | 0% | |
| 2,2-Dichloropropane | A | ug/L | 26.26917 | 1.0507668 | | 1 | 0 | 0 | 0.186 | 0.5 | 500 | 105% | 70 | 130 | 0% | |
| 2-Chlorotoluene | A | ug/L | 25.05504 | 1.0022016 | | 1 | 0 | 0 | 0.0876 | 0.5 | 500 | 100% | 70 | 130 | 0% | |
| 4-Chlorotoluene | A | ug/L | 24.39357 | 0.9757428 | | 1 | 0 | 0 | 0.0728 | 0.5 | 500 | 98% | 70 | 130 | 0% | |
| Benzene | A | ug/L | 23.79187 | 0.9516748 | | 1 | 0 | 0 | 0.0914 | 0.5 | 500 | 95% | 70 | 130 | 0% | |
| Bromobenzene | A | ug/L | 24.76128 | 0.9904512 | | 1 | 0 | 0 | 0.0831 | 0.5 | 500 | 99% | 70 | 130 | 0% | |
| Bromochloromethane | A | ug/L | 25.4383 | 1.017532 | | 1 | 0 | 0 | 0.141 | 0.5 | 500 | 102% | 70 | 130 | 0% | |
| Bromodichloromethane | A | ug/L | 24.39404 | 0.9757616 | | 1 | 0 | 0 | 0.12 | 0.5 | 500 | 98% | 70 | 130 | 0% | |
| Bromoform | A | ug/L | 25.92121 | 1.0368484 | | 1 | 0 | 0 | 0.119 | 0.5 | 500 | 104% | 70 | 130 | 0% | |
| Bromomethane | A | ug/L | 25.77927 | 1.0311708 | | 1 | 0 | 0 | 0.253 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| Carbon tetrachloride | A | ug/L | 24.77733 | 0.9910932 | | 1 | 0 | 0 | 0.143 | 0.5 | 500 | 99% | 70 | 130 | 0% | |
| Chlorobenzene | A | ug/L | 24.70152 | 0.9880608 | | 1 | 0 | 0 | 0.0914 | 0.5 | 500 | 99% | 70 | 130 | 0% | |
| Chlorodibromomethane | A | ug/L | 24.3492 | 0.973968 | | 1 | 0 | 0 | 0.0841 | 0.5 | 500 | 97% | 70 | 130 | 0% | |
| Chloroethane | A | ug/L | 26.12501 | 1.0450004 | | 1 | 0 | 0 | 0.169 | 0.5 | 500 | 105% | 70 | 130 | 0% | |
| Chloroform | A | ug/L | 24.17337 | 0.9669348 | | 1 | 0 | 0 | 0.0789 | 0.5 | 500 | 97% | 70 | 130 | 0% | |
| Chloromethane | A | ug/L | 26.34224 | 1.0536896 | | 1 | 0 | 0 | 0.162 | 0.5 | 500 | 105% | 70 | 130 | 0% | |
| cis-1,2-Dichloroethene | A | ug/L | 24.5653 | 0.982612 | | 1 | 0 | 0 | 0.108 | 0.5 | 500 | 98% | 70 | 130 | 0% | |
| cis-1,3-Dichloropropene | A | ug/L | 23.25283 | 0.9301132 | | 1 | 0 | 0 | 0.073 | 0.5 | 500 | 93% | 70 | 130 | 0% | |
| Dibromomethane | A | ug/L | 23.84392 | 0.9537568 | | 1 | 0 | 0 | 0.147 | 0.5 | 500 | 95% | 70 | 130 | 0% | |
| Dichlorodifluoromethane | A | ug/L | 25.67929 | 1.0271716 | | 1 | 0 | 0 | 0.175 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| Ethylbenzene | A | ug/L | 23.74212 | 0.9496848 | | 1 | 0 | 0 | 0.0836 | 0.5 | 500 | 95% | 70 | 130 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|--------------------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970902 | ICAL010422_3 | VOC-8260-W-Q | CAL3 | DA5975C\VG010 | 1/4/2022 4:28:05 | 1 | R372940 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| m+p-Xylenes | A | ug/L | 45.78355 | 1.831342 | | 2 | 0 | 0 | 0.15 | 0.5 | 1000 | 92% | 70 | 130 | 0% | |
| Methyl ethyl ketone | A | ug/L | 235.05043 | 9.4020172 | | 10 | 0 | 0 | 1.77 | 10 | 5000 | 94% | 70 | 130 | 0% | |
| Methyl tert-butyl ether (MTBE) | A | ug/L | 23.04184 | 0.9216736 | | 1 | 0 | 0 | 0.101 | 0.5 | 500 | 92% | 70 | 130 | 0% | |
| Methylene chloride | A | ug/L | 26.30581 | 1.0522324 | | 1 | 0 | 0 | 0.338 | 0.5 | 500 | 105% | 70 | 130 | 0% | |
| o-Xylene | A | ug/L | 23.64197 | 0.9456788 | | 1 | 0 | 0 | 0.0604 | 0.5 | 500 | 95% | 70 | 130 | 0% | |
| Styrene | A | ug/L | 23.41194 | 0.9364776 | | 1 | 0 | 0 | 0.067 | 0.5 | 500 | 94% | 70 | 130 | 0% | |
| Tetrachloroethene | A | ug/L | 25.39483 | 1.0157932 | | 1 | 0 | 0 | 0.0671 | 0.5 | 500 | 102% | 70 | 130 | 0% | |
| Toluene | A | ug/L | 23.63186 | 0.9452744 | | 1 | 0 | 0 | 0.0679 | 0.5 | 500 | 95% | 70 | 130 | 0% | |
| trans-1,2-Dichloroethene | A | ug/L | 25.46407 | 1.0185628 | | 1 | 0 | 0 | 0.125 | 0.5 | 500 | 102% | 70 | 130 | 0% | |
| trans-1,3-Dichloropropene | A | ug/L | 23.78943 | 0.9515772 | | 1 | 0 | 0 | 0.0846 | 0.5 | 500 | 95% | 70 | 130 | 0% | |
| Trichloroethene | A | ug/L | 24.14841 | 0.9659364 | | 1 | 0 | 0 | 0.0993 | 0.5 | 500 | 97% | 70 | 130 | 0% | |
| Trichlorofluoromethane | A | ug/L | 26.65307 | 1.0661228 | | 1 | 0 | 0 | 0.134 | 0.5 | 500 | 107% | 70 | 130 | 0% | |
| Vinyl chloride | A | ug/L | 25.64884 | 1.0259536 | | 1 | 0 | 0 | 0.153 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| 1,4-Dichlorobenzene-d4 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 70 | 130 | 0% | |
| Chlorobenzene-d5 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 70 | 130 | 0% | |
| Fluorobenzene | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 70 | 130 | 0% | |
| Xylenes, Total | M | ug/L | 69.42552 | 2.7770208 | | 3 | 0 | 0 | 0.0604 | 0.5 | 1500 | 93% | 70 | 130 | 0% | |
| 1,2-Dichloroethane-d4 | S | ug/L | 25.72803 | 1.0291212 | | 1 | 0 | 0 | 0.229 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| Dibromofluoromethane | S | ug/L | 25.62188 | 1.0248752 | | 1 | 0 | 0 | 0.129 | 0.5 | 500 | 102% | 70 | 130 | 0% | |
| p-Bromofluorobenzene | S | ug/L | 25.28989 | 1.0115956 | | 1 | 0 | 0 | 0.149 | 0.5 | 500 | 101% | 70 | 130 | 0% | |
| Toluene-d8 | S | ug/L | 23.3046 | 0.932184 | | 1 | 0 | 0 | 0.23 | 0.5 | 500 | 93% | 70 | 130 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970904 | ICAL010422_4 | VOC-8260-W-Q | CAL4 | DA5975C\VG010 | 1/4/2022 4:55:32 | 1 | R372940 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A | ug/L | 47.50287 | 1.9001148 | | 2 | 0 | 0 | 0.101 | 0.5 | 500 | 95% | 70 | 130 | 0% | |
| 1,1,1-Trichloroethane | A | ug/L | 48.26875 | 1.93075 | | 2 | 0 | 0 | 0.131 | 0.5 | 500 | 97% | 70 | 130 | 0% | |
| 1,1,2,2-Tetrachloroethane | A | ug/L | 48.61239 | 1.9444956 | | 2 | 0 | 0 | 0.0872 | 0.5 | 500 | 97% | 70 | 130 | 0% | |
| 1,1,2-Trichloroethane | A | ug/L | 48.47589 | 1.9390356 | | 2 | 0 | 0 | 0.108 | 0.5 | 500 | 97% | 70 | 130 | 0% | |
| 1,1-Dichloroethane | A | ug/L | 49.18279 | 1.9673116 | | 2 | 0 | 0 | 0.135 | 0.5 | 500 | 98% | 70 | 130 | 0% | |
| 1,1-Dichloroethene | A | ug/L | 48.80561 | 1.9522244 | | 2 | 0 | 0 | 0.141 | 0.5 | 500 | 98% | 70 | 130 | 0% | |
| 1,1-Dichloropropene | A | ug/L | 47.76266 | 1.9105064 | | 2 | 0 | 0 | 0.083 | 0.5 | 500 | 96% | 70 | 130 | 0% | |
| 1,2,3-Trichloropropane | A | ug/L | 49.19244 | 1.9676976 | | 2 | 0 | 0 | 0.235 | 0.5 | 500 | 98% | 70 | 130 | 0% | |
| 1,2-Dibromoethane | A | ug/L | 49.38886 | 1.9755544 | | 2 | 0 | 0 | 0.0916 | 0.5 | 500 | 99% | 70 | 130 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|--------------------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970904 | ICAL010422_4 | VOC-8260-W-Q | CAL4 | DA5975C\VG010 | 1/4/2022 4:55:32 | 1 | R372940 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,2-Dichlorobenzene | A | ug/L | 48.54976 | 1.9419904 | | 2 | 0 | 0 | 0.0746 | 0.5 | 500 | 97% | 70 | 130 | 0% | |
| 1,2-Dichloroethane | A | ug/L | 48.98798 | 1.9595192 | | 2 | 0 | 0 | 0.116 | 0.5 | 500 | 98% | 70 | 130 | 0% | |
| 1,2-Dichloropropane | A | ug/L | 47.52725 | 1.90109 | | 2 | 0 | 0 | 0.0847 | 0.5 | 500 | 95% | 70 | 130 | 0% | |
| 1,3-Dichlorobenzene | A | ug/L | 47.38535 | 1.895414 | | 2 | 0 | 0 | 0.0803 | 0.5 | 500 | 95% | 70 | 130 | 0% | |
| 1,3-Dichloropropane | A | ug/L | 48.8841 | 1.955364 | | 2 | 0 | 0 | 0.0791 | 0.5 | 500 | 98% | 70 | 130 | 0% | |
| 1,4-Dichlorobenzene | A | ug/L | 48.01064 | 1.9204256 | | 2 | 0 | 0 | 0.0858 | 0.5 | 500 | 96% | 70 | 130 | 0% | |
| 2,2-Dichloropropane | A | ug/L | 50.38039 | 2.0152156 | | 2 | 0 | 0 | 0.186 | 0.5 | 500 | 101% | 70 | 130 | 0% | |
| 2-Chlorotoluene | A | ug/L | 47.44663 | 1.8978652 | | 2 | 0 | 0 | 0.0876 | 0.5 | 500 | 95% | 70 | 130 | 0% | |
| 4-Chlorotoluene | A | ug/L | 48.3865 | 1.93546 | | 2 | 0 | 0 | 0.0728 | 0.5 | 500 | 97% | 70 | 130 | 0% | |
| Benzene | A | ug/L | 48.00539 | 1.9202156 | | 2 | 0 | 0 | 0.0914 | 0.5 | 500 | 96% | 70 | 130 | 0% | |
| Bromobenzene | A | ug/L | 47.5759 | 1.903036 | | 2 | 0 | 0 | 0.0831 | 0.5 | 500 | 95% | 70 | 130 | 0% | |
| Bromochloromethane | A | ug/L | 51.62325 | 2.06493 | | 2 | 0 | 0 | 0.141 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| Bromodichloromethane | A | ug/L | 47.2409 | 1.889636 | | 2 | 0 | 0 | 0.12 | 0.5 | 500 | 94% | 70 | 130 | 0% | |
| Bromoform | A | ug/L | 50.51704 | 2.0206816 | | 2 | 0 | 0 | 0.119 | 0.5 | 500 | 101% | 70 | 130 | 0% | |
| Bromomethane | A | ug/L | 47.59212 | 1.9036848 | | 2 | 0 | 0 | 0.253 | 0.5 | 500 | 95% | 70 | 130 | 0% | |
| Carbon tetrachloride | A | ug/L | 47.75203 | 1.9100812 | | 2 | 0 | 0 | 0.143 | 0.5 | 500 | 96% | 70 | 130 | 0% | |
| Chlorobenzene | A | ug/L | 47.39593 | 1.8958372 | | 2 | 0 | 0 | 0.0914 | 0.5 | 500 | 95% | 70 | 130 | 0% | |
| Chlorodibromomethane | A | ug/L | 46.24113 | 1.8496452 | | 2 | 0 | 0 | 0.0841 | 0.5 | 500 | 92% | 70 | 130 | 0% | |
| Chloroethane | A | ug/L | 46.22429 | 1.8489716 | | 2 | 0 | 0 | 0.169 | 0.5 | 500 | 92% | 70 | 130 | 0% | |
| Chloroform | A | ug/L | 48.20314 | 1.9281256 | | 2 | 0 | 0 | 0.0789 | 0.5 | 500 | 96% | 70 | 130 | 0% | |
| Chloromethane | A | ug/L | 49.79828 | 1.9919312 | | 2 | 0 | 0 | 0.162 | 0.5 | 500 | 100% | 70 | 130 | 0% | |
| cis-1,2-Dichloroethene | A | ug/L | 48.41535 | 1.936614 | | 2 | 0 | 0 | 0.108 | 0.5 | 500 | 97% | 70 | 130 | 0% | |
| cis-1,3-Dichloropropene | A | ug/L | 46.52826 | 1.8611304 | | 2 | 0 | 0 | 0.073 | 0.5 | 500 | 93% | 70 | 130 | 0% | |
| Dibromomethane | A | ug/L | 47.4844 | 1.899376 | | 2 | 0 | 0 | 0.147 | 0.5 | 500 | 95% | 70 | 130 | 0% | |
| Dichlorodifluoromethane | A | ug/L | 49.48348 | 1.9793392 | | 2 | 0 | 0 | 0.175 | 0.5 | 500 | 99% | 70 | 130 | 0% | |
| Ethylbenzene | A | ug/L | 46.80795 | 1.872318 | | 2 | 0 | 0 | 0.0836 | 0.5 | 500 | 94% | 70 | 130 | 0% | |
| m+p-Xylenes | A | ug/L | 92.53468 | 3.7013872 | | 4 | 0 | 0 | 0.15 | 0.5 | 1000 | 93% | 70 | 130 | 0% | |
| Methyl ethyl ketone | A | ug/L | 479.42958 | 19.1771832 | | 20 | 0 | 0 | 1.77 | 10 | 5000 | 96% | 70 | 130 | 0% | |
| Methyl tert-butyl ether (MTBE) | A | ug/L | 47.53006 | 1.9012024 | | 2 | 0 | 0 | 0.101 | 0.5 | 500 | 95% | 70 | 130 | 0% | |
| Methylene chloride | A | ug/L | 50.44212 | 2.0176848 | | 2 | 0 | 0 | 0.338 | 0.5 | 500 | 101% | 70 | 130 | 0% | |
| o-Xylene | A | ug/L | 47.5086 | 1.900344 | | 2 | 0 | 0 | 0.0604 | 0.5 | 500 | 95% | 70 | 130 | 0% | |
| Styrene | A | ug/L | 46.70518 | 1.8682072 | | 2 | 0 | 0 | 0.067 | 0.5 | 500 | 93% | 70 | 130 | 0% | |
| Tetrachloroethene | A | ug/L | 46.29317 | 1.8517268 | | 2 | 0 | 0 | 0.0671 | 0.5 | 500 | 93% | 70 | 130 | 0% | |
| Toluene | A | ug/L | 47.01163 | 1.8804652 | | 2 | 0 | 0 | 0.0679 | 0.5 | 500 | 94% | 70 | 130 | 0% | |
| trans-1,2-Dichloroethene | A | ug/L | 49.51777 | 1.9807108 | | 2 | 0 | 0 | 0.125 | 0.5 | 500 | 99% | 70 | 130 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970904 | ICAL010422_4 | VOC-8260-W-Q | CAL4 | DA5975C\VG010 | 1/4/2022 4:55:32 | 1 | R372940 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| trans-1,3-Dichloropropene | A | ug/L | 47.0378 | 1.881512 | | 2 | 0 | 0 | 0.0846 | 0.5 | 500 | 94% | 70 | 130 | 0% | |
| Trichloroethene | A | ug/L | 47.11894 | 1.8847576 | | 2 | 0 | 0 | 0.0993 | 0.5 | 500 | 94% | 70 | 130 | 0% | |
| Trichlorofluoromethane | A | ug/L | 49.31283 | 1.9725132 | | 2 | 0 | 0 | 0.134 | 0.5 | 500 | 99% | 70 | 130 | 0% | |
| Vinyl chloride | A | ug/L | 48.95796 | 1.9583184 | | 2 | 0 | 0 | 0.153 | 0.5 | 500 | 98% | 70 | 130 | 0% | |
| 1,4-Dichlorobenzene-d4 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 70 | 130 | 0% | |
| Chlorobenzene-d5 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 70 | 130 | 0% | |
| Fluorobenzene | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 70 | 130 | 0% | |
| Xylenes, Total | M | ug/L | 140.04328 | 5.6017312 | | 6 | 0 | 0 | 0.0604 | 0.5 | 1500 | 93% | 70 | 130 | 0% | |
| 1,2-Dichloroethane-d4 | S | ug/L | 48.12519 | 1.9250076 | | 2 | 0 | 0 | 0.229 | 0.5 | 500 | 96% | 70 | 130 | 0% | |
| Dibromofluoromethane | S | ug/L | 48.16607 | 1.9266428 | | 2 | 0 | 0 | 0.129 | 0.5 | 500 | 96% | 70 | 130 | 0% | |
| p-Bromofluorobenzene | S | ug/L | 46.6647 | 1.866588 | | 2 | 0 | 0 | 0.149 | 0.5 | 500 | 93% | 70 | 130 | 0% | |
| Toluene-d8 | S | ug/L | 47.14406 | 1.8857624 | | 2 | 0 | 0 | 0.23 | 0.5 | 500 | 94% | 70 | 130 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970905 | ICAL010422_5 | VOC-8260-W-Q | CAL5 | DA5975C\VG010 | 1/4/2022 5:50:25 | 1 | R372940 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A | ug/L | 119.0492 | 4.761968 | | 5 | 0 | 0 | 0.101 | 0.5 | 500 | 95% | 70 | 130 | 0% | |
| 1,1,1-Trichloroethane | A | ug/L | 118.57641 | 4.7430564 | | 5 | 0 | 0 | 0.131 | 0.5 | 500 | 95% | 70 | 130 | 0% | |
| 1,1,2,2-Tetrachloroethane | A | ug/L | 115.61793 | 4.6247172 | | 5 | 0 | 0 | 0.0872 | 0.5 | 500 | 92% | 70 | 130 | 0% | |
| 1,1,2-Trichloroethane | A | ug/L | 117.41297 | 4.6965188 | | 5 | 0 | 0 | 0.108 | 0.5 | 500 | 94% | 70 | 130 | 0% | |
| 1,1-Dichloroethane | A | ug/L | 118.11254 | 4.7245016 | | 5 | 0 | 0 | 0.135 | 0.5 | 500 | 94% | 70 | 130 | 0% | |
| 1,1-Dichloroethene | A | ug/L | 119.87977 | 4.7951908 | | 5 | 0 | 0 | 0.141 | 0.5 | 500 | 96% | 70 | 130 | 0% | |
| 1,1-Dichloropropene | A | ug/L | 119.80016 | 4.7920064 | | 5 | 0 | 0 | 0.083 | 0.5 | 500 | 96% | 70 | 130 | 0% | |
| 1,2,3-Trichloropropane | A | ug/L | 112.62609 | 4.5050436 | | 5 | 0 | 0 | 0.235 | 0.5 | 500 | 90% | 70 | 130 | 0% | |
| 1,2-Dibromoethane | A | ug/L | 119.23942 | 4.7695768 | | 5 | 0 | 0 | 0.0916 | 0.5 | 500 | 95% | 70 | 130 | 0% | |
| 1,2-Dichlorobenzene | A | ug/L | 115.43227 | 4.6172908 | | 5 | 0 | 0 | 0.0746 | 0.5 | 500 | 92% | 70 | 130 | 0% | |
| 1,2-Dichloroethane | A | ug/L | 118.21434 | 4.7285736 | | 5 | 0 | 0 | 0.116 | 0.5 | 500 | 95% | 70 | 130 | 0% | |
| 1,2-Dichloropropane | A | ug/L | 121.98902 | 4.8795608 | | 5 | 0 | 0 | 0.0847 | 0.5 | 500 | 98% | 70 | 130 | 0% | |
| 1,3-Dichlorobenzene | A | ug/L | 117.4899 | 4.699596 | | 5 | 0 | 0 | 0.0803 | 0.5 | 500 | 94% | 70 | 130 | 0% | |
| 1,3-Dichloropropane | A | ug/L | 123.01316 | 4.9205264 | | 5 | 0 | 0 | 0.0791 | 0.5 | 500 | 98% | 70 | 130 | 0% | |
| 1,4-Dichlorobenzene | A | ug/L | 118.7699 | 4.750796 | | 5 | 0 | 0 | 0.0858 | 0.5 | 500 | 95% | 70 | 130 | 0% | |
| 2,2-Dichloropropane | A | ug/L | 118.32027 | 4.7328108 | | 5 | 0 | 0 | 0.186 | 0.5 | 500 | 95% | 70 | 130 | 0% | |
| 2-Chlorotoluene | A | ug/L | 120.26748 | 4.8106992 | | 5 | 0 | 0 | 0.0876 | 0.5 | 500 | 96% | 70 | 130 | 0% | |
| 4-Chlorotoluene | A | ug/L | 121.05908 | 4.8423632 | | 5 | 0 | 0 | 0.0728 | 0.5 | 500 | 97% | 70 | 130 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|--------------------------------|--------------|--------------|------------|--------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970905 | ICAL010422_5 | VOC-8260-W-Q | CAL5 | DA5975CVG010 | 1/4/2022 5:50:25 | 1 | R372940 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| Benzene | A | ug/L | 116.95526 | 4.6782104 | | 5 | 0 | 0 | 0.0914 | 0.5 | 500 | 94% | 70 | 130 | 0% | |
| Bromobenzene | A | ug/L | 119.48008 | 4.7792032 | | 5 | 0 | 0 | 0.0831 | 0.5 | 500 | 96% | 70 | 130 | 0% | |
| Bromochloromethane | A | ug/L | 118.06829 | 4.7227316 | | 5 | 0 | 0 | 0.141 | 0.5 | 500 | 94% | 70 | 130 | 0% | |
| Bromodichloromethane | A | ug/L | 121.97488 | 4.8789952 | | 5 | 0 | 0 | 0.12 | 0.5 | 500 | 98% | 70 | 130 | 0% | |
| Bromoform | A | ug/L | 115.7218 | 4.628872 | | 5 | 0 | 0 | 0.119 | 0.5 | 500 | 93% | 70 | 130 | 0% | |
| Bromomethane | A | ug/L | 123.65037 | 4.9460148 | | 5 | 0 | 0 | 0.253 | 0.5 | 500 | 99% | 70 | 130 | 0% | |
| Carbon tetrachloride | A | ug/L | 119.4667 | 4.778668 | | 5 | 0 | 0 | 0.143 | 0.5 | 500 | 96% | 70 | 130 | 0% | |
| Chlorobenzene | A | ug/L | 120.69031 | 4.8276124 | | 5 | 0 | 0 | 0.0914 | 0.5 | 500 | 97% | 70 | 130 | 0% | |
| Chlorodibromomethane | A | ug/L | 120.74537 | 4.8298148 | | 5 | 0 | 0 | 0.0841 | 0.5 | 500 | 97% | 70 | 130 | 0% | |
| Chloroethane | A | ug/L | 122.40855 | 4.896342 | | 5 | 0 | 0 | 0.169 | 0.5 | 500 | 98% | 70 | 130 | 0% | |
| Chloroform | A | ug/L | 114.59119 | 4.5836476 | | 5 | 0 | 0 | 0.0789 | 0.5 | 500 | 92% | 70 | 130 | 0% | |
| Chloromethane | A | ug/L | 122.61785 | 4.904714 | | 5 | 0 | 0 | 0.162 | 0.5 | 500 | 98% | 70 | 130 | 0% | |
| cis-1,2-Dichloroethene | A | ug/L | 116.61895 | 4.664758 | | 5 | 0 | 0 | 0.108 | 0.5 | 500 | 93% | 70 | 130 | 0% | |
| cis-1,3-Dichloropropene | A | ug/L | 120.71159 | 4.8284636 | | 5 | 0 | 0 | 0.073 | 0.5 | 500 | 97% | 70 | 130 | 0% | |
| Dibromomethane | A | ug/L | 118.24252 | 4.7297008 | | 5 | 0 | 0 | 0.147 | 0.5 | 500 | 95% | 70 | 130 | 0% | |
| Dichlorodifluoromethane | A | ug/L | 127.81927 | 5.1127708 | | 5 | 0 | 0 | 0.175 | 0.5 | 500 | 102% | 70 | 130 | 0% | |
| Ethylbenzene | A | ug/L | 122.52434 | 4.9009736 | | 5 | 0 | 0 | 0.0836 | 0.5 | 500 | 98% | 70 | 130 | 0% | |
| m+p-Xylenes | A | ug/L | 250.25869 | 10.0103476 | | 10 | 0 | 0 | 0.15 | 0.5 | 1000 | 100% | 70 | 130 | 0% | |
| Methyl ethyl ketone | A | ug/L | 1159.30194 | 46.3720776 | | 50 | 0 | 0 | 1.77 | 10 | 5000 | 93% | 70 | 130 | 0% | |
| Methyl tert-butyl ether (MTBE) | A | ug/L | 127.13745 | 5.085498 | | 5 | 0 | 0 | 0.101 | 0.5 | 500 | 102% | 70 | 130 | 0% | |
| Methylene chloride | A | ug/L | 110.6249 | 4.424996 | | 5 | 0 | 0 | 0.338 | 0.5 | 500 | 88% | 70 | 130 | 0% | |
| o-Xylene | A | ug/L | 123.23778 | 4.9295112 | | 5 | 0 | 0 | 0.0604 | 0.5 | 500 | 99% | 70 | 130 | 0% | |
| Styrene | A | ug/L | 127.19102 | 5.0876408 | | 5 | 0 | 0 | 0.067 | 0.5 | 500 | 102% | 70 | 130 | 0% | |
| Tetrachloroethene | A | ug/L | 119.90031 | 4.7960124 | | 5 | 0 | 0 | 0.0671 | 0.5 | 500 | 96% | 70 | 130 | 0% | |
| Toluene | A | ug/L | 122.65711 | 4.9062844 | | 5 | 0 | 0 | 0.0679 | 0.5 | 500 | 98% | 70 | 130 | 0% | |
| trans-1,2-Dichloroethene | A | ug/L | 118.65107 | 4.7460428 | | 5 | 0 | 0 | 0.125 | 0.5 | 500 | 95% | 70 | 130 | 0% | |
| trans-1,3-Dichloropropene | A | ug/L | 121.49288 | 4.8597152 | | 5 | 0 | 0 | 0.0846 | 0.5 | 500 | 97% | 70 | 130 | 0% | |
| Trichloroethene | A | ug/L | 123.46463 | 4.9385852 | | 5 | 0 | 0 | 0.0993 | 0.5 | 500 | 99% | 70 | 130 | 0% | |
| Trichlorofluoromethane | A | ug/L | 129.06871 | 5.1627484 | | 5 | 0 | 0 | 0.134 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| Vinyl chloride | A | ug/L | 125.88087 | 5.0352348 | | 5 | 0 | 0 | 0.153 | 0.5 | 500 | 101% | 70 | 130 | 0% | |
| 1,4-Dichlorobenzene-d4 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 70 | 130 | 0% | |
| Chlorobenzene-d5 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 70 | 130 | 0% | |
| Fluorobenzene | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 70 | 130 | 0% | |
| Xylenes, Total | M | ug/L | 373.49647 | 14.9398588 | | 15 | 0 | 0 | 0.0604 | 0.5 | 1500 | 100% | 70 | 130 | 0% | |
| 1,2-Dichloroethane-d4 | S | ug/L | 116.64203 | 4.6656812 | | 5 | 0 | 0 | 0.229 | 0.5 | 500 | 93% | 70 | 130 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|----------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970905 | ICAL010422_5 | VOC-8260-W-Q | CAL5 | DA5975C\VG010 | 1/4/2022 5:50:25 | 1 | R372940 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| Dibromofluoromethane | S | ug/L | 115.11464 | 4.6045856 | | 5 | 0 | 0 | 0.129 | 0.5 | 500 | 92% | 70 | 130 | 0% | |
| p-Bromofluorobenzene | S | ug/L | 117.93503 | 4.7174012 | | 5 | 0 | 0 | 0.149 | 0.5 | 500 | 94% | 70 | 130 | 0% | |
| Toluene-d8 | S | ug/L | 121.27495 | 4.850998 | | 5 | 0 | 0 | 0.23 | 0.5 | 500 | 97% | 70 | 130 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970906 | ICAL010422_6 | VOC-8260-W-Q | CAL6 | DA5975C\VG010 | 1/4/2022 6:45:10 | 1 | R372940 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A | ug/L | 254.82737 | 10.1930948 | | 10 | 0 | 0 | 0.101 | 0.5 | 500 | 102% | 70 | 130 | 0% | |
| 1,1,1-Trichloroethane | A | ug/L | 258.72281 | 10.3489124 | | 10 | 0 | 0 | 0.131 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| 1,1,2,2-Tetrachloroethane | A | ug/L | 250.15769 | 10.0063076 | | 10 | 0 | 0 | 0.0872 | 0.5 | 500 | 100% | 70 | 130 | 0% | |
| 1,1,2-Trichloroethane | A | ug/L | 248.28816 | 9.9315264 | | 10 | 0 | 0 | 0.108 | 0.5 | 500 | 99% | 70 | 130 | 0% | |
| 1,1-Dichloroethane | A | ug/L | 258.43252 | 10.3373008 | | 10 | 0 | 0 | 0.135 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| 1,1-Dichloroethene | A | ug/L | 258.09028 | 10.3236112 | | 10 | 0 | 0 | 0.141 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| 1,1-Dichloropropene | A | ug/L | 264.6638 | 10.586552 | | 10 | 0 | 0 | 0.083 | 0.5 | 500 | 106% | 70 | 130 | 0% | |
| 1,2,3-Trichloropropane | A | ug/L | 249.26347 | 9.9705388 | | 10 | 0 | 0 | 0.235 | 0.5 | 500 | 100% | 70 | 130 | 0% | |
| 1,2-Dibromoethane | A | ug/L | 257.88869 | 10.3155476 | | 10 | 0 | 0 | 0.0916 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| 1,2-Dichlorobenzene | A | ug/L | 257.65242 | 10.3060968 | | 10 | 0 | 0 | 0.0746 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| 1,2-Dichloroethane | A | ug/L | 251.96754 | 10.0787016 | | 10 | 0 | 0 | 0.116 | 0.5 | 500 | 101% | 70 | 130 | 0% | |
| 1,2-Dichloropropane | A | ug/L | 254.71606 | 10.1886424 | | 10 | 0 | 0 | 0.0847 | 0.5 | 500 | 102% | 70 | 130 | 0% | |
| 1,3-Dichlorobenzene | A | ug/L | 258.62971 | 10.3451884 | | 10 | 0 | 0 | 0.0803 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| 1,3-Dichloropropane | A | ug/L | 263.47539 | 10.5390156 | | 10 | 0 | 0 | 0.0791 | 0.5 | 500 | 105% | 70 | 130 | 0% | |
| 1,4-Dichlorobenzene | A | ug/L | 254.91697 | 10.1966788 | | 10 | 0 | 0 | 0.0858 | 0.5 | 500 | 102% | 70 | 130 | 0% | |
| 2,2-Dichloropropane | A | ug/L | 253.03965 | 10.121586 | | 10 | 0 | 0 | 0.186 | 0.5 | 500 | 101% | 70 | 130 | 0% | |
| 2-Chlorotoluene | A | ug/L | 267.26165 | 10.690466 | | 10 | 0 | 0 | 0.0876 | 0.5 | 500 | 107% | 70 | 130 | 0% | |
| 4-Chlorotoluene | A | ug/L | 267.44092 | 10.6976368 | | 10 | 0 | 0 | 0.0728 | 0.5 | 500 | 107% | 70 | 130 | 0% | |
| Benzene | A | ug/L | 257.54165 | 10.301666 | | 10 | 0 | 0 | 0.0914 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| Bromobenzene | A | ug/L | 263.29438 | 10.5317752 | | 10 | 0 | 0 | 0.0831 | 0.5 | 500 | 105% | 70 | 130 | 0% | |
| Bromochloromethane | A | ug/L | 247.05862 | 9.8823448 | | 10 | 0 | 0 | 0.141 | 0.5 | 500 | 99% | 70 | 130 | 0% | |
| Bromodichloromethane | A | ug/L | 257.22856 | 10.2891424 | | 10 | 0 | 0 | 0.12 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| Bromoform | A | ug/L | 257.5099 | 10.300396 | | 10 | 0 | 0 | 0.119 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| Bromomethane | A | ug/L | 251.76065 | 10.070426 | | 10 | 0 | 0 | 0.253 | 0.5 | 500 | 101% | 70 | 130 | 0% | |
| Carbon tetrachloride | A | ug/L | 260.87744 | 10.4350976 | | 10 | 0 | 0 | 0.143 | 0.5 | 500 | 104% | 70 | 130 | 0% | |
| Chlorobenzene | A | ug/L | 258.25445 | 10.330178 | | 10 | 0 | 0 | 0.0914 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| Chlorodibromomethane | A | ug/L | 258.35353 | 10.3341412 | | 10 | 0 | 0 | 0.0841 | 0.5 | 500 | 103% | 70 | 130 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|--------------------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970906 | ICAL010422_6 | VOC-8260-W-Q | CAL6 | DA5975C\VG010 | 1/4/2022 6:45:10 | 1 | R372940 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| Chloroethane | A | ug/L | 231.74321 | 9.2697284 | | 10 | 0 | 0 | 0.169 | 0.5 | 500 | 93% | 70 | 130 | 0% | |
| Chloroform | A | ug/L | 248.08043 | 9.9232172 | | 10 | 0 | 0 | 0.0789 | 0.5 | 500 | 99% | 70 | 130 | 0% | |
| Chloromethane | A | ug/L | 240.2183 | 9.608732 | | 10 | 0 | 0 | 0.162 | 0.5 | 500 | 96% | 70 | 130 | 0% | |
| cis-1,2-Dichloroethene | A | ug/L | 261.87064 | 10.4748256 | | 10 | 0 | 0 | 0.108 | 0.5 | 500 | 105% | 70 | 130 | 0% | |
| cis-1,3-Dichloropropene | A | ug/L | 265.28626 | 10.6114504 | | 10 | 0 | 0 | 0.073 | 0.5 | 500 | 106% | 70 | 130 | 0% | |
| Dibromomethane | A | ug/L | 252.27336 | 10.0909344 | | 10 | 0 | 0 | 0.147 | 0.5 | 500 | 101% | 70 | 130 | 0% | |
| Dichlorodifluoromethane | A | ug/L | 252.15586 | 10.0862344 | | 10 | 0 | 0 | 0.175 | 0.5 | 500 | 101% | 70 | 130 | 0% | |
| Ethylbenzene | A | ug/L | 266.81931 | 10.6727724 | | 10 | 0 | 0 | 0.0836 | 0.5 | 500 | 107% | 70 | 130 | 0% | |
| m+p-Xylenes | A | ug/L | 543.42617 | 21.7370468 | | 20 | 0 | 0 | 0.15 | 0.5 | 1000 | 109% | 70 | 130 | 0% | |
| Methyl ethyl ketone | A | ug/L | 2688.24739 | 107.529896 | | 100 | 0 | 0 | 1.77 | 10 | 5000 | 108% | 70 | 130 | 0% | |
| Methyl tert-butyl ether (MTBE) | A | ug/L | 258.95351 | 10.3581404 | | 10 | 0 | 0 | 0.101 | 0.5 | 500 | 104% | 70 | 130 | 0% | |
| Methylene chloride | A | ug/L | 235.46573 | 9.4186292 | | 10 | 0 | 0 | 0.338 | 0.5 | 500 | 94% | 70 | 130 | 0% | |
| o-Xylene | A | ug/L | 270.46357 | 10.8185428 | | 10 | 0 | 0 | 0.0604 | 0.5 | 500 | 108% | 70 | 130 | 0% | |
| Styrene | A | ug/L | 278.0455 | 11.12182 | | 10 | 0 | 0 | 0.067 | 0.5 | 500 | 111% | 70 | 130 | 0% | |
| Tetrachloroethene | A | ug/L | 259.74185 | 10.389674 | | 10 | 0 | 0 | 0.0671 | 0.5 | 500 | 104% | 70 | 130 | 0% | |
| Toluene | A | ug/L | 263.13299 | 10.5253196 | | 10 | 0 | 0 | 0.0679 | 0.5 | 500 | 105% | 70 | 130 | 0% | |
| trans-1,2-Dichloroethene | A | ug/L | 254.6608 | 10.186432 | | 10 | 0 | 0 | 0.125 | 0.5 | 500 | 102% | 70 | 130 | 0% | |
| trans-1,3-Dichloropropene | A | ug/L | 263.80268 | 10.5521072 | | 10 | 0 | 0 | 0.0846 | 0.5 | 500 | 106% | 70 | 130 | 0% | |
| Trichloroethene | A | ug/L | 262.29307 | 10.4917228 | | 10 | 0 | 0 | 0.0993 | 0.5 | 500 | 105% | 70 | 130 | 0% | |
| Trichlorofluoromethane | A | ug/L | 259.05024 | 10.3620096 | | 10 | 0 | 0 | 0.134 | 0.5 | 500 | 104% | 70 | 130 | 0% | |
| Vinyl chloride | A | ug/L | 248.65325 | 9.94613 | | 10 | 0 | 0 | 0.153 | 0.5 | 500 | 99% | 70 | 130 | 0% | |
| 1,4-Dichlorobenzene-d4 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 70 | 130 | 0% | |
| Chlorobenzene-d5 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 70 | 130 | 0% | |
| Fluorobenzene | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 70 | 130 | 0% | |
| Xylenes, Total | M | ug/L | 813.88974 | 32.5555896 | | 30 | 0 | 0 | 0.0604 | 0.5 | 1500 | 109% | 70 | 130 | 0% | |
| 1,2-Dichloroethane-d4 | S | ug/L | 258.23239 | 10.3292956 | | 10 | 0 | 0 | 0.229 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| Dibromofluoromethane | S | ug/L | 259.02233 | 10.3608932 | | 10 | 0 | 0 | 0.129 | 0.5 | 500 | 104% | 70 | 130 | 0% | |
| p-Bromofluorobenzene | S | ug/L | 267.31855 | 10.692742 | | 10 | 0 | 0 | 0.149 | 0.5 | 500 | 107% | 70 | 130 | 0% | |
| Toluene-d8 | S | ug/L | 270.0265 | 10.80106 | | 10 | 0 | 0 | 0.23 | 0.5 | 500 | 108% | 70 | 130 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|----------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970907 | ICAL010422_7 | VOC-8260-W-Q | CAL7 | DA5975C\VG010 | 1/4/2022 7:39:45 | 1 | R372940 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970907 | ICAL010422_7 | VOC-8260-W-Q | CAL7 | DA5975C\VG010 | 1/4/2022 7:39:45 | 1 | R372940 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A | ug/L | 392.18595 | 15.687438 | | 15 | 0 | 0 | 0.101 | 0.5 | 500 | 105% | 70 | 130 | 0% | |
| 1,1,1-Trichloroethane | A | ug/L | 386.6625 | 15.4665 | | 15 | 0 | 0 | 0.131 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| 1,1,2,2-Tetrachloroethane | A | ug/L | 367.42759 | 14.6971036 | | 15 | 0 | 0 | 0.0872 | 0.5 | 500 | 98% | 70 | 130 | 0% | |
| 1,1,2-Trichloroethane | A | ug/L | 373.25341 | 14.9301364 | | 15 | 0 | 0 | 0.108 | 0.5 | 500 | 100% | 70 | 130 | 0% | |
| 1,1-Dichloroethane | A | ug/L | 380.44366 | 15.2177464 | | 15 | 0 | 0 | 0.135 | 0.5 | 500 | 101% | 70 | 130 | 0% | |
| 1,1-Dichloroethene | A | ug/L | 380.37253 | 15.2149012 | | 15 | 0 | 0 | 0.141 | 0.5 | 500 | 101% | 70 | 130 | 0% | |
| 1,1-Dichloropropene | A | ug/L | 397.13223 | 15.8852892 | | 15 | 0 | 0 | 0.083 | 0.5 | 500 | 106% | 70 | 130 | 0% | |
| 1,2,3-Trichloropropane | A | ug/L | 363.67316 | 14.5469264 | | 15 | 0 | 0 | 0.235 | 0.5 | 500 | 97% | 70 | 130 | 0% | |
| 1,2-Dibromoethane | A | ug/L | 377.7698 | 15.110792 | | 15 | 0 | 0 | 0.0916 | 0.5 | 500 | 101% | 70 | 130 | 0% | |
| 1,2-Dichlorobenzene | A | ug/L | 375.32826 | 15.0131304 | | 15 | 0 | 0 | 0.0746 | 0.5 | 500 | 100% | 70 | 130 | 0% | |
| 1,2-Dichloroethane | A | ug/L | 366.9787 | 14.679148 | | 15 | 0 | 0 | 0.116 | 0.5 | 500 | 98% | 70 | 130 | 0% | |
| 1,2-Dichloropropane | A | ug/L | 388.85021 | 15.5540084 | | 15 | 0 | 0 | 0.0847 | 0.5 | 500 | 104% | 70 | 130 | 0% | |
| 1,3-Dichlorobenzene | A | ug/L | 383.62247 | 15.3448988 | | 15 | 0 | 0 | 0.0803 | 0.5 | 500 | 102% | 70 | 130 | 0% | |
| 1,3-Dichloropropane | A | ug/L | 389.34421 | 15.5737684 | | 15 | 0 | 0 | 0.0791 | 0.5 | 500 | 104% | 70 | 130 | 0% | |
| 1,4-Dichlorobenzene | A | ug/L | 371.39689 | 14.8558756 | | 15 | 0 | 0 | 0.0858 | 0.5 | 500 | 99% | 70 | 130 | 0% | |
| 2,2-Dichloropropane | A | ug/L | 369.84356 | 14.7937424 | | 15 | 0 | 0 | 0.186 | 0.5 | 500 | 99% | 70 | 130 | 0% | |
| 2-Chlorotoluene | A | ug/L | 391.82688 | 15.6730752 | | 15 | 0 | 0 | 0.0876 | 0.5 | 500 | 104% | 70 | 130 | 0% | |
| 4-Chlorotoluene | A | ug/L | 396.27563 | 15.8510252 | | 15 | 0 | 0 | 0.0728 | 0.5 | 500 | 106% | 70 | 130 | 0% | |
| Benzene | A | ug/L | 385.85261 | 15.4341044 | | 15 | 0 | 0 | 0.0914 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| Bromobenzene | A | ug/L | 386.44198 | 15.4576792 | | 15 | 0 | 0 | 0.0831 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| Bromochloromethane | A | ug/L | 371.80037 | 14.8720148 | | 15 | 0 | 0 | 0.141 | 0.5 | 500 | 99% | 70 | 130 | 0% | |
| Bromodichloromethane | A | ug/L | 386.19404 | 15.4477616 | | 15 | 0 | 0 | 0.12 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| Bromoform | A | ug/L | 378.22002 | 15.1288008 | | 15 | 0 | 0 | 0.119 | 0.5 | 500 | 101% | 70 | 130 | 0% | |
| Bromomethane | A | ug/L | 385.12594 | 15.4050376 | | 15 | 0 | 0 | 0.253 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| Carbon tetrachloride | A | ug/L | 386.9014 | 15.476056 | | 15 | 0 | 0 | 0.143 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| Chlorobenzene | A | ug/L | 386.94547 | 15.4778188 | | 15 | 0 | 0 | 0.0914 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| Chlorodibromomethane | A | ug/L | 387.68121 | 15.5072484 | | 15 | 0 | 0 | 0.0841 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| Chloroethane | A | ug/L | 364.45728 | 14.5782912 | | 15 | 0 | 0 | 0.169 | 0.5 | 500 | 97% | 70 | 130 | 0% | |
| Chloroform | A | ug/L | 366.93889 | 14.6775556 | | 15 | 0 | 0 | 0.0789 | 0.5 | 500 | 98% | 70 | 130 | 0% | |
| Chloromethane | A | ug/L | 352.08363 | 14.0833452 | | 15 | 0 | 0 | 0.162 | 0.5 | 500 | 94% | 70 | 130 | 0% | |
| cis-1,2-Dichloroethene | A | ug/L | 386.72365 | 15.468946 | | 15 | 0 | 0 | 0.108 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| cis-1,3-Dichloropropene | A | ug/L | 400.79296 | 16.0317184 | | 15 | 0 | 0 | 0.073 | 0.5 | 500 | 107% | 70 | 130 | 0% | |
| Dibromomethane | A | ug/L | 380.65469 | 15.2261876 | | 15 | 0 | 0 | 0.147 | 0.5 | 500 | 102% | 70 | 130 | 0% | |
| Dichlorodifluoromethane | A | ug/L | 373.94485 | 14.957794 | | 15 | 0 | 0 | 0.175 | 0.5 | 500 | 100% | 70 | 130 | 0% | |
| Ethylbenzene | A | ug/L | 404.7587 | 16.190348 | | 15 | 0 | 0 | 0.0836 | 0.5 | 500 | 108% | 70 | 130 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|--------------------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970907 | ICAL010422_7 | VOC-8260-W-Q | CAL7 | DA5975C\VG010 | 1/4/2022 7:39:45 | 1 | R372940 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| m+p-Xylenes | A | ug/L | 812.85557 | 32.5142228 | | 30 | 0 | 0 | 0.15 | 0.5 | 1000 | 108% | 70 | 130 | 0% | |
| Methyl ethyl ketone | A | ug/L | 3961.341 | 158.45364 | | 150 | 0 | 0 | 1.77 | 10 | 5000 | 106% | 70 | 130 | 0% | |
| Methyl tert-butyl ether (MTBE) | A | ug/L | 391.17667 | 15.6470668 | | 15 | 0 | 0 | 0.101 | 0.5 | 500 | 104% | 70 | 130 | 0% | |
| Methylene chloride | A | ug/L | 348.06663 | 13.9226652 | | 15 | 0 | 0 | 0.338 | 0.5 | 500 | 93% | 70 | 130 | 0% | |
| o-Xylene | A | ug/L | 408.20432 | 16.3281728 | | 15 | 0 | 0 | 0.0604 | 0.5 | 500 | 109% | 70 | 130 | 0% | |
| Styrene | A | ug/L | 413.75947 | 16.5503788 | | 15 | 0 | 0 | 0.067 | 0.5 | 500 | 110% | 70 | 130 | 0% | |
| Tetrachloroethene | A | ug/L | 382.87963 | 15.3151852 | | 15 | 0 | 0 | 0.0671 | 0.5 | 500 | 102% | 70 | 130 | 0% | |
| Toluene | A | ug/L | 397.01061 | 15.8804244 | | 15 | 0 | 0 | 0.0679 | 0.5 | 500 | 106% | 70 | 130 | 0% | |
| trans-1,2-Dichloroethene | A | ug/L | 376.13673 | 15.0454692 | | 15 | 0 | 0 | 0.125 | 0.5 | 500 | 100% | 70 | 130 | 0% | |
| trans-1,3-Dichloropropene | A | ug/L | 402.10977 | 16.0843908 | | 15 | 0 | 0 | 0.0846 | 0.5 | 500 | 107% | 70 | 130 | 0% | |
| Trichloroethene | A | ug/L | 394.48959 | 15.7795836 | | 15 | 0 | 0 | 0.0993 | 0.5 | 500 | 105% | 70 | 130 | 0% | |
| Trichlorofluoromethane | A | ug/L | 371.42899 | 14.8571596 | | 15 | 0 | 0 | 0.134 | 0.5 | 500 | 99% | 70 | 130 | 0% | |
| Vinyl chloride | A | ug/L | 372.35639 | 14.8942556 | | 15 | 0 | 0 | 0.153 | 0.5 | 500 | 99% | 70 | 130 | 0% | |
| 1,4-Dichlorobenzene-d4 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 70 | 130 | 0% | |
| Chlorobenzene-d5 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 70 | 130 | 0% | |
| Fluorobenzene | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 70 | 130 | 0% | |
| Xylenes, Total | M | ug/L | 1221.05989 | 48.8423956 | | 45 | 0 | 0 | 0.0604 | 0.5 | 1500 | 109% | 70 | 130 | 0% | |
| 1,2-Dichloroethane-d4 | S | ug/L | 378.33349 | 15.1333396 | | 15 | 0 | 0 | 0.229 | 0.5 | 500 | 101% | 70 | 130 | 0% | |
| Dibromofluoromethane | S | ug/L | 384.7503 | 15.390012 | | 15 | 0 | 0 | 0.129 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| p-Bromofluorobenzene | S | ug/L | 394.65655 | 15.786262 | | 15 | 0 | 0 | 0.149 | 0.5 | 500 | 105% | 70 | 130 | 0% | |
| Toluene-d8 | S | ug/L | 405.5583 | 16.222332 | | 15 | 0 | 0 | 0.23 | 0.5 | 500 | 108% | 70 | 130 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970908 | ICAL010422_8 | VOC-8260-W-Q | CAL8 | DA5975C\VG010 | 1/4/2022 8:34:31 | 1 | R372940 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A | ug/L | 520.28551 | 20.8114204 | | 20 | 0 | 0 | 0.101 | 0.5 | 500 | 104% | 70 | 130 | 0% | |
| 1,1,1-Trichloroethane | A | ug/L | 518.83124 | 20.7532496 | | 20 | 0 | 0 | 0.131 | 0.5 | 500 | 104% | 70 | 130 | 0% | |
| 1,1,2,2-Tetrachloroethane | A | ug/L | 491.66999 | 19.6667996 | | 20 | 0 | 0 | 0.0872 | 0.5 | 500 | 98% | 70 | 130 | 0% | |
| 1,1,2-Trichloroethane | A | ug/L | 505.18031 | 20.2072124 | | 20 | 0 | 0 | 0.108 | 0.5 | 500 | 101% | 70 | 130 | 0% | |
| 1,1-Dichloroethane | A | ug/L | 515.3207 | 20.612828 | | 20 | 0 | 0 | 0.135 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| 1,1-Dichloroethene | A | ug/L | 515.06031 | 20.6024124 | | 20 | 0 | 0 | 0.141 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| 1,1-Dichloropropene | A | ug/L | 543.51208 | 21.7404832 | | 20 | 0 | 0 | 0.083 | 0.5 | 500 | 109% | 70 | 130 | 0% | |
| 1,2,3-Trichloropropane | A | ug/L | 491.52294 | 19.6609176 | | 20 | 0 | 0 | 0.235 | 0.5 | 500 | 98% | 70 | 130 | 0% | |
| 1,2-Dibromoethane | A | ug/L | 507.9234 | 20.316936 | | 20 | 0 | 0 | 0.0916 | 0.5 | 500 | 102% | 70 | 130 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|--------------------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970908 | ICAL010422_8 | VOC-8260-W-Q | CAL8 | DA5975C\VG010 | 1/4/2022 8:34:31 | 1 | R372940 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,2-Dichlorobenzene | A | ug/L | 506.38707 | 20.2554828 | | 20 | 0 | 0 | 0.0746 | 0.5 | 500 | 101% | 70 | 130 | 0% | |
| 1,2-Dichloroethane | A | ug/L | 497.36991 | 19.8947964 | | 20 | 0 | 0 | 0.116 | 0.5 | 500 | 99% | 70 | 130 | 0% | |
| 1,2-Dichloropropane | A | ug/L | 524.16945 | 20.966778 | | 20 | 0 | 0 | 0.0847 | 0.5 | 500 | 105% | 70 | 130 | 0% | |
| 1,3-Dichlorobenzene | A | ug/L | 511.55042 | 20.4620168 | | 20 | 0 | 0 | 0.0803 | 0.5 | 500 | 102% | 70 | 130 | 0% | |
| 1,3-Dichloropropane | A | ug/L | 511.24793 | 20.4499172 | | 20 | 0 | 0 | 0.0791 | 0.5 | 500 | 102% | 70 | 130 | 0% | |
| 1,4-Dichlorobenzene | A | ug/L | 502.30007 | 20.0920028 | | 20 | 0 | 0 | 0.0858 | 0.5 | 500 | 100% | 70 | 130 | 0% | |
| 2,2-Dichloropropane | A | ug/L | 499.04726 | 19.9618904 | | 20 | 0 | 0 | 0.186 | 0.5 | 500 | 100% | 70 | 130 | 0% | |
| 2-Chlorotoluene | A | ug/L | 538.49638 | 21.5398552 | | 20 | 0 | 0 | 0.0876 | 0.5 | 500 | 108% | 70 | 130 | 0% | |
| 4-Chlorotoluene | A | ug/L | 531.84706 | 21.2738824 | | 20 | 0 | 0 | 0.0728 | 0.5 | 500 | 106% | 70 | 130 | 0% | |
| Benzene | A | ug/L | 511.66576 | 20.4666304 | | 20 | 0 | 0 | 0.0914 | 0.5 | 500 | 102% | 70 | 130 | 0% | |
| Bromobenzene | A | ug/L | 516.0104 | 20.640416 | | 20 | 0 | 0 | 0.0831 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| Bromochloromethane | A | ug/L | 494.60544 | 19.7842176 | | 20 | 0 | 0 | 0.141 | 0.5 | 500 | 99% | 70 | 130 | 0% | |
| Bromodichloromethane | A | ug/L | 518.37176 | 20.7348704 | | 20 | 0 | 0 | 0.12 | 0.5 | 500 | 104% | 70 | 130 | 0% | |
| Bromoform | A | ug/L | 522.76605 | 20.910642 | | 20 | 0 | 0 | 0.119 | 0.5 | 500 | 105% | 70 | 130 | 0% | |
| Bromomethane | A | ug/L | 515.01414 | 20.6005656 | | 20 | 0 | 0 | 0.253 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| Carbon tetrachloride | A | ug/L | 521.26297 | 20.8505188 | | 20 | 0 | 0 | 0.143 | 0.5 | 500 | 104% | 70 | 130 | 0% | |
| Chlorobenzene | A | ug/L | 515.99575 | 20.63983 | | 20 | 0 | 0 | 0.0914 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| Chlorodibromomethane | A | ug/L | 520.43607 | 20.8174428 | | 20 | 0 | 0 | 0.0841 | 0.5 | 500 | 104% | 70 | 130 | 0% | |
| Chloroethane | A | ug/L | 481.51432 | 19.2605728 | | 20 | 0 | 0 | 0.169 | 0.5 | 500 | 96% | 70 | 130 | 0% | |
| Chloroform | A | ug/L | 489.12212 | 19.5648848 | | 20 | 0 | 0 | 0.0789 | 0.5 | 500 | 98% | 70 | 130 | 0% | |
| Chloromethane | A | ug/L | 480.17469 | 19.2069876 | | 20 | 0 | 0 | 0.162 | 0.5 | 500 | 96% | 70 | 130 | 0% | |
| cis-1,2-Dichloroethene | A | ug/L | 516.05445 | 20.642178 | | 20 | 0 | 0 | 0.108 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| cis-1,3-Dichloropropene | A | ug/L | 538.90085 | 21.556034 | | 20 | 0 | 0 | 0.073 | 0.5 | 500 | 108% | 70 | 130 | 0% | |
| Dibromomethane | A | ug/L | 500.74556 | 20.0298224 | | 20 | 0 | 0 | 0.147 | 0.5 | 500 | 100% | 70 | 130 | 0% | |
| Dichlorodifluoromethane | A | ug/L | 494.74738 | 19.7898952 | | 20 | 0 | 0 | 0.175 | 0.5 | 500 | 99% | 70 | 130 | 0% | |
| Ethylbenzene | A | ug/L | 544.68805 | 21.787522 | | 20 | 0 | 0 | 0.0836 | 0.5 | 500 | 109% | 70 | 130 | 0% | |
| m+p-Xylenes | A | ug/L | 1087.40818 | 43.4963272 | | 40 | 0 | 0 | 0.15 | 0.5 | 1000 | 109% | 70 | 130 | 0% | |
| Methyl ethyl ketone | A | ug/L | 5327.12526 | 213.085010 | | 200 | 0 | 0 | 1.77 | 10 | 5000 | 107% | 70 | 130 | 0% | |
| Methyl tert-butyl ether (MTBE) | A | ug/L | 522.81865 | 20.912746 | | 20 | 0 | 0 | 0.101 | 0.5 | 500 | 105% | 70 | 130 | 0% | |
| Methylene chloride | A | ug/L | 466.99932 | 18.6799728 | | 20 | 0 | 0 | 0.338 | 0.5 | 500 | 93% | 70 | 130 | 0% | |
| o-Xylene | A | ug/L | 547.47638 | 21.8990552 | | 20 | 0 | 0 | 0.0604 | 0.5 | 500 | 109% | 70 | 130 | 0% | |
| Styrene | A | ug/L | 555.79455 | 22.231782 | | 20 | 0 | 0 | 0.067 | 0.5 | 500 | 111% | 70 | 130 | 0% | |
| Tetrachloroethene | A | ug/L | 514.92548 | 20.5970192 | | 20 | 0 | 0 | 0.0671 | 0.5 | 500 | 103% | 70 | 130 | 0% | |
| Toluene | A | ug/L | 536.51007 | 21.4604028 | | 20 | 0 | 0 | 0.0679 | 0.5 | 500 | 107% | 70 | 130 | 0% | |
| trans-1,2-Dichloroethene | A | ug/L | 510.00974 | 20.4003896 | | 20 | 0 | 0 | 0.125 | 0.5 | 500 | 102% | 70 | 130 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970908 | ICAL010422_8 | VOC-8260-W-Q | CAL8 | DA5975C\VG010 | 1/4/2022 8:34:31 | 1 | R372940 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| trans-1,3-Dichloropropene | A | ug/L | 533.75507 | 21.3502028 | | 20 | 0 | 0 | 0.0846 | 0.5 | 500 | 107% | 70 | 130 | 0% | |
| Trichloroethene | A | ug/L | 534.40073 | 21.3760292 | | 20 | 0 | 0 | 0.0993 | 0.5 | 500 | 107% | 70 | 130 | 0% | |
| Trichlorofluoromethane | A | ug/L | 489.6475 | 19.5859 | | 20 | 0 | 0 | 0.134 | 0.5 | 500 | 98% | 70 | 130 | 0% | |
| Vinyl chloride | A | ug/L | 498.3563 | 19.934252 | | 20 | 0 | 0 | 0.153 | 0.5 | 500 | 100% | 70 | 130 | 0% | |
| 1,4-Dichlorobenzene-d4 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 70 | 130 | 0% | |
| Chlorobenzene-d5 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 70 | 130 | 0% | |
| Fluorobenzene | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 70 | 130 | 0% | |
| Xylenes, Total | M | ug/L | 1634.88456 | 65.3953824 | | 60 | 0 | 0 | 0.0604 | 0.5 | 1500 | 109% | 70 | 130 | 0% | |
| 1,2-Dichloroethane-d4 | S | ug/L | 510.30803 | 20.4123212 | | 20 | 0 | 0 | 0.229 | 0.5 | 500 | 102% | 70 | 130 | 0% | |
| Dibromofluoromethane | S | ug/L | 510.39915 | 20.415966 | | 20 | 0 | 0 | 0.129 | 0.5 | 500 | 102% | 70 | 130 | 0% | |
| p-Bromofluorobenzene | S | ug/L | 541.3964 | 21.655856 | | 20 | 0 | 0 | 0.149 | 0.5 | 500 | 108% | 70 | 130 | 0% | |
| Toluene-d8 | S | ug/L | 544.21357 | 21.7685428 | | 20 | 0 | 0 | 0.23 | 0.5 | 500 | 109% | 70 | 130 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|-----------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970909 | ICV010422 | VOC-8260-W-Q | ICV | DA5975C\VG010 | 1/4/2022 9:29:14 | 1 | R372940 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A | ug/L | 126.66575 | 5.06663 | | 5 | 0 | 0 | 0.101 | 0.5 | 500 | 101% | 80 | 120 | 0% | |
| 1,1,1-Trichloroethane | A | ug/L | 128.25238 | 5.1300952 | | 5 | 0 | 0 | 0.131 | 0.5 | 500 | 103% | 80 | 120 | 0% | |
| 1,1,2,2-Tetrachloroethane | A | ug/L | 127.47217 | 5.0988868 | | 5 | 0 | 0 | 0.0872 | 0.5 | 500 | 102% | 80 | 120 | 0% | |
| 1,1,2-Trichloroethane | A | ug/L | 123.03611 | 4.9214444 | | 5 | 0 | 0 | 0.108 | 0.5 | 500 | 98% | 80 | 120 | 0% | |
| 1,1-Dichloroethane | A | ug/L | 135.803 | 5.43212 | | 5 | 0 | 0 | 0.135 | 0.5 | 500 | 109% | 80 | 120 | 0% | |
| 1,1-Dichloroethene | A | ug/L | 134.45663 | 5.3782652 | | 5 | 0 | 0 | 0.141 | 0.5 | 500 | 108% | 80 | 120 | 0% | |
| 1,1-Dichloropropene | A | ug/L | 124.18526 | 4.9674104 | | 5 | 0 | 0 | 0.083 | 0.5 | 500 | 99% | 80 | 120 | 0% | |
| 1,2,3-Trichloropropane | A | ug/L | 122.95232 | 4.9180928 | | 5 | 0 | 0 | 0.235 | 0.5 | 500 | 98% | 80 | 120 | 0% | |
| 1,2-Dibromoethane | A | ug/L | 124.27642 | 4.9710568 | | 5 | 0 | 0 | 0.0916 | 0.5 | 500 | 99% | 80 | 120 | 0% | |
| 1,2-Dichlorobenzene | A | ug/L | 128.71039 | 5.1484156 | | 5 | 0 | 0 | 0.0746 | 0.5 | 500 | 103% | 80 | 120 | 0% | |
| 1,2-Dichloroethane | A | ug/L | 120.79914 | 4.8319656 | | 5 | 0 | 0 | 0.116 | 0.5 | 500 | 97% | 80 | 120 | 0% | |
| 1,2-Dichloropropane | A | ug/L | 125.66265 | 5.026506 | | 5 | 0 | 0 | 0.0847 | 0.5 | 500 | 101% | 80 | 120 | 0% | |
| 1,3-Dichlorobenzene | A | ug/L | 135.11854 | 5.4047416 | | 5 | 0 | 0 | 0.0803 | 0.5 | 500 | 108% | 80 | 120 | 0% | |
| 1,3-Dichloropropane | A | ug/L | 121.84417 | 4.8737668 | | 5 | 0 | 0 | 0.0791 | 0.5 | 500 | 97% | 80 | 120 | 0% | |
| 1,4-Dichlorobenzene | A | ug/L | 129.88123 | 5.1952492 | | 5 | 0 | 0 | 0.0858 | 0.5 | 500 | 104% | 80 | 120 | 0% | |
| 2,2-Dichloropropane | A | ug/L | 131.40305 | 5.256122 | | 5 | 0 | 0 | 0.186 | 0.5 | 500 | 105% | 80 | 120 | 0% | |
| 2-Chlorotoluene | A | ug/L | 131.29475 | 5.25179 | | 5 | 0 | 0 | 0.0876 | 0.5 | 500 | 105% | 80 | 120 | 0% | |
| 4-Chlorotoluene | A | ug/L | 137.07902 | 5.4831608 | | 5 | 0 | 0 | 0.0728 | 0.5 | 500 | 110% | 80 | 120 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|--------------------------------|-----------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970909 | ICV010422 | VOC-8260-W-Q | ICV | DA5975C\VG010 | 1/4/2022 9:29:14 | 1 | R372940 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| Benzene | A | ug/L | 131.31393 | 5.2525572 | | 5 | 0 | 0 | 0.0914 | 0.5 | 500 | 105% | 80 | 120 | 0% | |
| Bromobenzene | A | ug/L | 131.67879 | 5.2671516 | | 5 | 0 | 0 | 0.0831 | 0.5 | 500 | 105% | 80 | 120 | 0% | |
| Bromochloromethane | A | ug/L | 123.60094 | 4.9440376 | | 5 | 0 | 0 | 0.141 | 0.5 | 500 | 99% | 80 | 120 | 0% | |
| Bromodichloromethane | A | ug/L | 128.87588 | 5.1550352 | | 5 | 0 | 0 | 0.12 | 0.5 | 500 | 103% | 80 | 120 | 0% | |
| Bromoform | A | ug/L | 129.9644 | 5.198576 | | 5 | 0 | 0 | 0.119 | 0.5 | 500 | 104% | 80 | 120 | 0% | |
| Bromomethane | A | ug/L | 116.91567 | 4.6766268 | | 5 | 0 | 0 | 0.253 | 0.5 | 500 | 94% | 80 | 120 | 0% | |
| Carbon tetrachloride | A | ug/L | 128.79275 | 5.15171 | | 5 | 0 | 0 | 0.143 | 0.5 | 500 | 103% | 80 | 120 | 0% | |
| Chlorobenzene | A | ug/L | 131.63517 | 5.2654068 | | 5 | 0 | 0 | 0.0914 | 0.5 | 500 | 105% | 80 | 120 | 0% | |
| Chlorodibromomethane | A | ug/L | 125.11031 | 5.0044124 | | 5 | 0 | 0 | 0.0841 | 0.5 | 500 | 100% | 80 | 120 | 0% | |
| Chloroethane | A | ug/L | 115.59324 | 4.6237296 | | 5 | 0 | 0 | 0.169 | 0.5 | 500 | 92% | 80 | 120 | 0% | |
| Chloroform | A | ug/L | 120.42358 | 4.8169432 | | 5 | 0 | 0 | 0.0789 | 0.5 | 500 | 96% | 80 | 120 | 0% | |
| Chloromethane | A | ug/L | 108.77392 | 4.3509568 | | 5 | 0 | 0 | 0.162 | 0.5 | 500 | 87% | 80 | 120 | 0% | |
| cis-1,2-Dichloroethene | A | ug/L | 130.12309 | 5.2049236 | | 5 | 0 | 0 | 0.108 | 0.5 | 500 | 104% | 80 | 120 | 0% | |
| cis-1,3-Dichloropropene | A | ug/L | 121.55615 | 4.862246 | | 5 | 0 | 0 | 0.073 | 0.5 | 500 | 97% | 80 | 120 | 0% | |
| Dibromomethane | A | ug/L | 125.30472 | 5.0121888 | | 5 | 0 | 0 | 0.147 | 0.5 | 500 | 100% | 80 | 120 | 0% | |
| Dichlorodifluoromethane | A | ug/L | 111.37489 | 4.4549956 | | 5 | 0 | 0 | 0.175 | 0.5 | 500 | 89% | 80 | 120 | 0% | |
| Ethylbenzene | A | ug/L | 131.91134 | 5.2764536 | | 5 | 0 | 0 | 0.0836 | 0.5 | 500 | 106% | 80 | 120 | 0% | |
| m+p-Xylenes | A | ug/L | 262.75886 | 10.5103544 | | 10 | 0 | 0 | 0.15 | 0.5 | 1000 | 105% | 80 | 120 | 0% | |
| Methyl ethyl ketone | A | ug/L | 1198.44392 | 47.9377568 | | 50 | 0 | 0 | 1.77 | 10 | 5000 | 96% | 80 | 120 | 0% | |
| Methyl tert-butyl ether (MTBE) | A | ug/L | 134.72237 | 5.3888948 | | 5 | 0 | 0 | 0.101 | 0.5 | 500 | 108% | 80 | 120 | 0% | |
| Methylene chloride | A | ug/L | 121.52968 | 4.8611872 | | 5 | 0 | 0 | 0.338 | 0.5 | 500 | 97% | 80 | 120 | 0% | |
| o-Xylene | A | ug/L | 132.22141 | 5.2888564 | | 5 | 0 | 0 | 0.0604 | 0.5 | 500 | 106% | 80 | 120 | 0% | |
| Styrene | A | ug/L | 137.49736 | 5.4998944 | | 5 | 0 | 0 | 0.067 | 0.5 | 500 | 110% | 80 | 120 | 0% | |
| Tetrachloroethene | A | ug/L | 126.01413 | 5.0405652 | | 5 | 0 | 0 | 0.0671 | 0.5 | 500 | 101% | 80 | 120 | 0% | |
| Toluene | A | ug/L | 132.0244 | 5.280976 | | 5 | 0 | 0 | 0.0679 | 0.5 | 500 | 106% | 80 | 120 | 0% | |
| trans-1,2-Dichloroethene | A | ug/L | 134.70283 | 5.3881132 | | 5 | 0 | 0 | 0.125 | 0.5 | 500 | 108% | 80 | 120 | 0% | |
| trans-1,3-Dichloropropene | A | ug/L | 129.02156 | 5.1608624 | | 5 | 0 | 0 | 0.0846 | 0.5 | 500 | 103% | 80 | 120 | 0% | |
| Trichloroethene | A | ug/L | 131.10958 | 5.2443832 | | 5 | 0 | 0 | 0.0993 | 0.5 | 500 | 105% | 80 | 120 | 0% | |
| Trichlorofluoromethane | A | ug/L | 121.7847 | 4.871388 | | 5 | 0 | 0 | 0.134 | 0.5 | 500 | 97% | 80 | 120 | 0% | |
| Vinyl chloride | A | ug/L | 120.15175 | 4.80607 | | 5 | 0 | 0 | 0.153 | 0.5 | 500 | 96% | 80 | 120 | 0% | |
| 1,4-Dichlorobenzene-d4 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 0 | 0 | 0% | |
| Chlorobenzene-d5 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 0 | 0 | 0% | |
| Fluorobenzene | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 0 | 0 | 0% | |
| Xylenes, Total | M | ug/L | 394.98027 | 15.7992108 | | 15 | 0 | 0 | 0.0604 | 0.5 | 1500 | 105% | 80 | 120 | 0% | |
| 1,2-Dichloroethane-d4 | S | ug/L | 280.28858 | 11.2115432 | | 10 | 0 | 0 | 0.229 | 0.5 | 500 | 112% | 80 | 120 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|----------------------|-----------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970909 | ICV010422 | VOC-8260-W-Q | ICV | DA5975C\VG010 | 1/4/2022 9:29:14 | 1 | R372940 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| Dibromofluoromethane | S | ug/L | 271.19937 | 10.8479748 | | 10 | 0 | 0 | 0.129 | 0.5 | 500 | 108% | 80 | 120 | 0% | |
| p-Bromofluorobenzene | S | ug/L | 269.89759 | 10.7959036 | | 10 | 0 | 0 | 0.149 | 0.5 | 500 | 108% | 80 | 120 | 0% | |
| Toluene-d8 | S | ug/L | 276.91062 | 11.0764248 | | 10 | 0 | 0 | 0.23 | 0.5 | 500 | 111% | 80 | 120 | 0% | |

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN01.D
Sample Name : PRIMER
Operator : MSC
Date injected : 4 Jan 2022 9:44 am
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 1

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN02.D
Sample Name : BFB010422_
Operator : MSC
Date injected : 4 Jan 2022 10:11 am
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 2

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN03.D
Sample Name : CCV010422_
Operator : MSC
Date injected : 4 Jan 2022 10:56 am
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 3

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN04.D
Sample Name : PRIMER
Misc. Info. : Replaced purge trap
Operator : MSC
Date injected : 4 Jan 2022 12:17 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 4

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN05.D
Sample Name : BFB010422_

Operator : MSC
Date injected : 4 Jan 2022 12:44 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 5

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN06.D
Sample Name : CCV010422_
Operator : MSC
Date injected : 4 Jan 2022 1:24 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 6

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN07.D
Sample Name : BLK
Operator : MSC
Date injected : 4 Jan 2022 2:09 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.839
End Time : 16.498
Vial Number : 7

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN08.D
Sample Name : BFB010422_
Operator : MSC
Date injected : 4 Jan 2022 2:38 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 8

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN09.D
Sample Name : MBLK010422_
Operator : MSC
Date injected : 4 Jan 2022 3:05 pm
Instrument : VOA5975C

Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 9

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN10.D
Sample Name : ICAL010422_1
Operator : MSC
Date injected : 4 Jan 2022 3:33 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 10

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN11.D
Sample Name : ICAL010422_2
Operator : MSC
Date injected : 4 Jan 2022 4:00 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 11

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN12.D
Sample Name : ICAL010422_3
Operator : MSC
Date injected : 4 Jan 2022 4:28 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 12

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN13.D
Sample Name : ICAL010422_4
Operator : MSC
Date injected : 4 Jan 2022 4:55 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840

End Time : 16.498
Vial Number : 13

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN14.D
Sample Name : BLK
Operator : MSC
Date injected : 4 Jan 2022 5:22 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 14

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN15.D
Sample Name : ICAL010422_5
Operator : MSC
Date injected : 4 Jan 2022 5:50 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 15

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN16.D
Sample Name : BLK
Operator : MSC
Date injected : 4 Jan 2022 6:17 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 16

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN17.D
Sample Name : ICAL010422_6
Operator : MSC
Date injected : 4 Jan 2022 6:45 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 17

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN18.D
Sample Name : BLK
Operator : MSC
Date injected : 4 Jan 2022 7:12 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 18

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN19.D
Sample Name : ICAL010422_7
Operator : MSC
Date injected : 4 Jan 2022 7:39 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 19

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN20.D
Sample Name : BLK
Operator : MSC
Date injected : 4 Jan 2022 8:07 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.839
End Time : 16.498
Vial Number : 20

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN21.D
Sample Name : ICAL010422_8
Operator : MSC
Date injected : 4 Jan 2022 8:34 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 21

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN22.D
Sample Name : BLK

Operator : MSC
Date injected : 4 Jan 2022 9:01 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.839
End Time : 16.498
Vial Number : 22

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN23.D
Sample Name : ICV010422
Operator : MSC
Date injected : 4 Jan 2022 9:29 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 23

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN24.D
Sample Name : BLK
Operator : MSC
Date injected : 4 Jan 2022 9:56 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.839
End Time : 16.498
Vial Number : 24

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN25.D
Sample Name : MDL010422_Q1_1
Operator : MSC
Date injected : 4 Jan 2022 10:23 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 25

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN26.D
Sample Name : LOD010422_Q1_HalfCAL2
Operator : MSC
Date injected : 4 Jan 2022 10:51 pm
Instrument : VOA5975C



Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.839
End Time : 16.498
Vial Number : 26

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN27.D
Sample Name : MDL010422_Q1_2xCAL1
Operator : MSC
Date injected : 4 Jan 2022 11:18 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 27

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN28.D
Sample Name : BLK
Operator : MSC
Date injected : 4 Jan 2022 11:45 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 28

Tune Evaluation Report

Data Path: D:\Org\Data\VOA5975C\VG010422\04JAN08.D
 Acq on: 1/4/2022 2:38:09 PM
 Operator: MSC
 Sample: BFB010422_
 Inst Name: VOA5975C
 ALS Vial: 8
 Method: \\MASSHUNTER\Org\Data\Methods\BFBapex.m



| Target Mass | Rel. To Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|-----------|
| 50 | 95 | 15 | 40 | 21.2 | 51080 | Pass |
| 75 | 95 | 30 | 60 | 51.0 | 122824 | Pass |
| 95 | 95 | 100 | 100 | 100.0 | 240768 | Pass |
| 96 | 95 | 5 | 9 | 5.4 | 12961 | Pass |
| 173 | 174 | 0 | 2 | 0.0 | 0 | Pass |
| 174 | 95 | 50 | 100 | 95.2 | 229120 | Pass |
| 175 | 174 | 5 | 9 | 6.6 | 15102 | Pass |
| 176 | 174 | 95 | 101 | 95.7 | 219264 | Pass |
| 177 | 176 | 5 | 9 | 6.7 | 14796 | Pass |

Quantitative Analysis Results Summary Report

| | | | |
|---------------------|---|----------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:48 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

Sequence Table

| Data File | sample Name | Sample Type | Vial Position | Inj Vol | Level | Acq Method File |
|-----------|--------------|--------------|---------------|---------|-------|-----------------|
| 04JAN09.D | MBLK010422_ | Method Blank | 9 | 0 | | 5975CACQF.M |
| 04JAN10.D | ICAL010422_1 | Cal | 10 | 0 | 1 | 5975CACQF.M |
| 04JAN11.D | ICAL010422_2 | Cal | 11 | 0 | 2 | 5975CACQF.M |
| 04JAN12.D | ICAL010422_3 | Cal | 12 | 0 | 3 | 5975CACQF.M |
| 04JAN13.D | ICAL010422_4 | Cal | 13 | 0 | 4 | 5975CACQF.M |
| 04JAN15.D | ICAL010422_5 | Cal | 15 | 0 | 5 | 5975CACQF.M |
| 04JAN17.D | ICAL010422_6 | Cal | 17 | 0 | 6 | 5975CACQF.M |
| 04JAN19.D | ICAL010422_7 | Cal | 19 | 0 | 7 | 5975CACQF.M |
| 04JAN21.D | ICAL010422_8 | Cal | 21 | 0 | 8 | 5975CACQF.M |
| 04JAN23.D | ICV010422 | QC | 23 | 0 | QC | 5975CACQF.M |

Quantitation Results

Compound: Dichlorodifluoromethane

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Fluorobenzene | | | 775552 | | ND | | |
| 04JAN10.D | Calibration | Fluorobenzene | 1.241 | 4353 | 770895 | 0.0056 | 4.3090 | 2.5000 | 172.4 |
| 04JAN11.D | Calibration | Fluorobenzene | 1.244 | 12087 | 764419 | 0.0158 | 12.0663 | 12.5000 | 96.5 |
| 04JAN12.D | Calibration | Fluorobenzene | 1.244 | 26627 | 791270 | 0.0337 | 25.6793 | 25.0000 | 102.7 |
| 04JAN13.D | Calibration | Fluorobenzene | 1.241 | 50457 | 778120 | 0.0648 | 49.4835 | 50.0000 | 99.0 |
| 04JAN15.D | Calibration | Fluorobenzene | 1.241 | 137933 | 823488 | 0.1675 | 127.8193 | 125.0000 | 102.3 |
| 04JAN17.D | Calibration | Fluorobenzene | 1.241 | 276334 | 836278 | 0.3304 | 252.1559 | 250.0000 | 100.9 |
| 04JAN19.D | Calibration | Fluorobenzene | 1.241 | 412544 | 841876 | 0.4900 | 373.9449 | 375.0000 | 99.7 |
| 04JAN21.D | Calibration | Fluorobenzene | 1.241 | 545484 | 841364 | 0.6483 | 494.7474 | 500.0000 | 98.9 |
| 04JAN23.D | QC | Fluorobenzene | 1.241 | 116936 | 801210 | 0.1459 | 111.3749 | 125.0000 | |

Compound: Chloromethane

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Fluorobenzene | 1.333 | 0 | 775552 | 0.0000 | ND | | |
| 04JAN10.D | Calibration | Fluorobenzene | 1.406 | 7435 | 770895 | 0.0096 | 6.0637 | 2.5000 | 242.5 |
| 04JAN11.D | Calibration | Fluorobenzene | 1.406 | 16859 | 764419 | 0.0221 | 13.8661 | 12.5000 | 110.9 |
| 04JAN12.D | Calibration | Fluorobenzene | 1.406 | 33153 | 791270 | 0.0419 | 26.3422 | 25.0000 | 105.4 |
| 04JAN13.D | Calibration | Fluorobenzene | 1.408 | 61632 | 778120 | 0.0792 | 49.7983 | 50.0000 | 99.6 |
| 04JAN15.D | Calibration | Fluorobenzene | 1.409 | 160604 | 823488 | 0.1950 | 122.6179 | 125.0000 | 98.1 |
| 04JAN17.D | Calibration | Fluorobenzene | 1.408 | 319523 | 836278 | 0.3821 | 240.2183 | 250.0000 | 96.1 |
| 04JAN19.D | Calibration | Fluorobenzene | 1.409 | 471454 | 841876 | 0.5600 | 352.0836 | 375.0000 | 93.9 |
| 04JAN21.D | Calibration | Fluorobenzene | 1.406 | 642582 | 841364 | 0.7637 | 480.1747 | 500.0000 | 96.0 |

Quantitative Analysis Results Summary Report

Compound: Chloromethane

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN23.D | QC | Fluorobenzene | 1.406 | 138617 | 801210 | 0.1730 | 108.7739 | 125.0000 | |

Compound: Vinyl chloride

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Fluorobenzene | 1.489 | 0 | 775552 | 0.0000 | ND | | |
| 04JAN10.D | Calibration | Fluorobenzene | 1.495 | 4274 | 770895 | 0.0055 | 3.8739 | 2.5000 | 155.0 |
| 04JAN11.D | Calibration | Fluorobenzene | 1.498 | 13724 | 764419 | 0.0180 | 12.5446 | 12.5000 | 100.4 |
| 04JAN12.D | Calibration | Fluorobenzene | 1.495 | 29046 | 791270 | 0.0367 | 25.6488 | 25.0000 | 102.6 |
| 04JAN13.D | Calibration | Fluorobenzene | 1.495 | 54521 | 778120 | 0.0701 | 48.9580 | 50.0000 | 97.9 |
| 04JAN15.D | Calibration | Fluorobenzene | 1.495 | 148358 | 823488 | 0.1802 | 125.8809 | 125.0000 | 100.7 |
| 04JAN17.D | Calibration | Fluorobenzene | 1.498 | 297604 | 836278 | 0.3559 | 248.6532 | 250.0000 | 99.5 |
| 04JAN19.D | Calibration | Fluorobenzene | 1.498 | 448643 | 841876 | 0.5329 | 372.3564 | 375.0000 | 99.3 |
| 04JAN21.D | Calibration | Fluorobenzene | 1.495 | 600092 | 841364 | 0.7132 | 498.3563 | 500.0000 | 99.7 |
| 04JAN23.D | QC | Fluorobenzene | 1.495 | 137775 | 801210 | 0.1720 | 120.1518 | 125.0000 | |

Compound: Bromomethane

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Fluorobenzene | | | 775552 | | ND | | |
| 04JAN10.D | Calibration | Fluorobenzene | 1.796 | 1902 | 770895 | 0.0025 | 3.8547 | 2.5000 | 154.2 |
| 04JAN11.D | Calibration | Fluorobenzene | 1.796 | 5893 | 764419 | 0.0077 | 12.0464 | 12.5000 | 96.4 |
| 04JAN12.D | Calibration | Fluorobenzene | 1.796 | 13054 | 791270 | 0.0165 | 25.7793 | 25.0000 | 103.1 |
| 04JAN13.D | Calibration | Fluorobenzene | 1.799 | 23699 | 778120 | 0.0305 | 47.5921 | 50.0000 | 95.2 |
| 04JAN15.D | Calibration | Fluorobenzene | 1.799 | 65163 | 823488 | 0.0791 | 123.6504 | 125.0000 | 98.9 |
| 04JAN17.D | Calibration | Fluorobenzene | 1.799 | 134737 | 836278 | 0.1611 | 251.7606 | 250.0000 | 100.7 |
| 04JAN19.D | Calibration | Fluorobenzene | 1.796 | 207491 | 841876 | 0.2465 | 385.1259 | 375.0000 | 102.7 |
| 04JAN21.D | Calibration | Fluorobenzene | 1.793 | 277301 | 841364 | 0.3296 | 515.0141 | 500.0000 | 103.0 |
| 04JAN23.D | QC | Fluorobenzene | 1.796 | 59947 | 801210 | 0.0748 | 116.9157 | 125.0000 | |

Compound: Chloroethane

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Fluorobenzene | | | 775552 | | ND | | |
| 04JAN10.D | Calibration | Fluorobenzene | 1.899 | 2178 | 770895 | 0.0028 | 3.9871 | 2.5000 | 159.5 |
| 04JAN11.D | Calibration | Fluorobenzene | 1.897 | 8052 | 764419 | 0.0105 | 14.8670 | 12.5000 | 118.9 |
| 04JAN12.D | Calibration | Fluorobenzene | 1.897 | 14646 | 791270 | 0.0185 | 26.1250 | 25.0000 | 104.5 |
| 04JAN13.D | Calibration | Fluorobenzene | 1.897 | 25484 | 778120 | 0.0328 | 46.2243 | 50.0000 | 92.4 |
| 04JAN15.D | Calibration | Fluorobenzene | 1.894 | 71420 | 823488 | 0.0867 | 122.4086 | 125.0000 | 97.9 |
| 04JAN17.D | Calibration | Fluorobenzene | 1.894 | 137312 | 836278 | 0.1642 | 231.7432 | 250.0000 | 92.7 |
| 04JAN19.D | Calibration | Fluorobenzene | 1.897 | 217393 | 841876 | 0.2582 | 364.4573 | 375.0000 | 97.2 |
| 04JAN21.D | Calibration | Fluorobenzene | 1.894 | 287041 | 841364 | 0.3412 | 481.5143 | 500.0000 | 96.3 |
| 04JAN23.D | QC | Fluorobenzene | 1.897 | 65619 | 801210 | 0.0819 | 115.5932 | 125.0000 | |

Quantitative Analysis Results Summary Report

Compound: Trichlorofluoromethane

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Fluorobenzene | | | 775552 | | ND | | |
| 04JAN10.D | Calibration | Fluorobenzene | 2.153 | 5030 | 770895 | 0.0065 | 3.6731 | 2.5000 | 146.9 |
| 04JAN11.D | Calibration | Fluorobenzene | 2.142 | 15431 | 764419 | 0.0202 | 11.3637 | 12.5000 | 90.9 |
| 04JAN12.D | Calibration | Fluorobenzene | 2.142 | 37464 | 791270 | 0.0473 | 26.6531 | 25.0000 | 106.6 |
| 04JAN13.D | Calibration | Fluorobenzene | 2.145 | 68163 | 778120 | 0.0876 | 49.3128 | 50.0000 | 98.6 |
| 04JAN15.D | Calibration | Fluorobenzene | 2.142 | 188808 | 823488 | 0.2293 | 129.0687 | 125.0000 | 103.3 |
| 04JAN17.D | Calibration | Fluorobenzene | 2.145 | 384837 | 836278 | 0.4602 | 259.0502 | 250.0000 | 103.6 |
| 04JAN19.D | Calibration | Fluorobenzene | 2.145 | 555477 | 841876 | 0.6598 | 371.4290 | 375.0000 | 99.0 |
| 04JAN21.D | Calibration | Fluorobenzene | 2.145 | 731829 | 841364 | 0.8698 | 489.6475 | 500.0000 | 97.9 |
| 04JAN23.D | QC | Fluorobenzene | 2.145 | 173333 | 801210 | 0.2163 | 121.7847 | 125.0000 | |

Compound: 1,1-Dichloroethene

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Fluorobenzene | | | 775552 | | ND | | |
| 04JAN10.D | Calibration | Fluorobenzene | 2.700 | 2084 | 770895 | 0.0027 | 2.6839 | 2.5000 | 107.4 |
| 04JAN11.D | Calibration | Fluorobenzene | 2.700 | 9169 | 764419 | 0.0120 | 11.9081 | 12.5000 | 95.3 |
| 04JAN12.D | Calibration | Fluorobenzene | 2.700 | 20631 | 791270 | 0.0261 | 25.8849 | 25.0000 | 103.5 |
| 04JAN13.D | Calibration | Fluorobenzene | 2.702 | 38253 | 778120 | 0.0492 | 48.8056 | 50.0000 | 97.6 |
| 04JAN15.D | Calibration | Fluorobenzene | 2.697 | 99438 | 823488 | 0.1208 | 119.8798 | 125.0000 | 95.9 |
| 04JAN17.D | Calibration | Fluorobenzene | 2.702 | 217406 | 836278 | 0.2600 | 258.0903 | 250.0000 | 103.2 |
| 04JAN19.D | Calibration | Fluorobenzene | 2.700 | 322557 | 841876 | 0.3831 | 380.3725 | 375.0000 | 101.4 |
| 04JAN21.D | Calibration | Fluorobenzene | 2.700 | 436507 | 841364 | 0.5188 | 515.0603 | 500.0000 | 103.0 |
| 04JAN23.D | QC | Fluorobenzene | 2.702 | 108512 | 801210 | 0.1354 | 134.4566 | 125.0000 | |

Compound: Methylene chloride

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Fluorobenzene | 3.335 | 1661 | 775552 | 0.0021 | 1.4424 | | |
| 04JAN10.D | Calibration | Fluorobenzene | 3.324 | 4095 | 770895 | 0.0053 | 3.5774 | 2.5000 | 143.1 |
| 04JAN11.D | Calibration | Fluorobenzene | 3.338 | 17734 | 764419 | 0.0232 | 15.6236 | 12.5000 | 125.0 |
| 04JAN12.D | Calibration | Fluorobenzene | 3.333 | 30908 | 791270 | 0.0391 | 26.3058 | 25.0000 | 105.2 |
| 04JAN13.D | Calibration | Fluorobenzene | 3.335 | 58282 | 778120 | 0.0749 | 50.4421 | 50.0000 | 100.9 |
| 04JAN15.D | Calibration | Fluorobenzene | 3.336 | 135271 | 823488 | 0.1643 | 110.6249 | 125.0000 | 88.5 |
| 04JAN17.D | Calibration | Fluorobenzene | 3.333 | 292397 | 836278 | 0.3496 | 235.4657 | 250.0000 | 94.2 |
| 04JAN19.D | Calibration | Fluorobenzene | 3.330 | 435116 | 841876 | 0.5168 | 348.0666 | 375.0000 | 92.8 |
| 04JAN21.D | Calibration | Fluorobenzene | 3.330 | 583438 | 841364 | 0.6934 | 466.9993 | 500.0000 | 93.4 |
| 04JAN23.D | QC | Fluorobenzene | 3.330 | 144585 | 801210 | 0.1805 | 121.5297 | 125.0000 | |

Compound: trans-1,2-Dichloroethene

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Fluorobenzene | | | 775552 | | ND | | |
| 04JAN10.D | Calibration | Fluorobenzene | 3.723 | 2146 | 770895 | 0.0028 | 2.7090 | 2.5000 | 108.4 |
| 04JAN11.D | Calibration | Fluorobenzene | 3.720 | 9821 | 764419 | 0.0128 | 12.5022 | 12.5000 | 100.0 |

Quantitative Analysis Results Summary Report

Compound: trans-1,2-Dichloroethene

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN12.D | Calibration | Fluorobenzene | 3.712 | 20706 | 791270 | 0.0262 | 25.4641 | 25.0000 | 101.9 |
| 04JAN13.D | Calibration | Fluorobenzene | 3.717 | 39596 | 778120 | 0.0509 | 49.5178 | 50.0000 | 99.0 |
| 04JAN15.D | Calibration | Fluorobenzene | 3.718 | 100409 | 823488 | 0.1219 | 118.6511 | 125.0000 | 94.9 |
| 04JAN17.D | Calibration | Fluorobenzene | 3.715 | 218855 | 836278 | 0.2617 | 254.6608 | 250.0000 | 101.9 |
| 04JAN19.D | Calibration | Fluorobenzene | 3.715 | 325415 | 841876 | 0.3865 | 376.1367 | 375.0000 | 100.3 |
| 04JAN21.D | Calibration | Fluorobenzene | 3.718 | 440967 | 841364 | 0.5241 | 510.0097 | 500.0000 | 102.0 |
| 04JAN23.D | QC | Fluorobenzene | 3.715 | 110909 | 801210 | 0.1384 | 134.7028 | 125.0000 | |

Compound: Methyl tert-butyl ether (MTBE)

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Fluorobenzene | | | 775552 | | ND | | |
| 04JAN10.D | Calibration | Fluorobenzene | 3.759 | 2717 | 770895 | 0.0035 | 2.6532 | 2.5000 | 106.1 |
| 04JAN11.D | Calibration | Fluorobenzene | 3.762 | 12515 | 764419 | 0.0164 | 12.3255 | 12.5000 | 98.6 |
| 04JAN12.D | Calibration | Fluorobenzene | 3.754 | 24218 | 791270 | 0.0306 | 23.0418 | 25.0000 | 92.2 |
| 04JAN13.D | Calibration | Fluorobenzene | 3.757 | 49126 | 778120 | 0.0631 | 47.5301 | 50.0000 | 95.1 |
| 04JAN15.D | Calibration | Fluorobenzene | 3.754 | 139068 | 823488 | 0.1689 | 127.1375 | 125.0000 | 101.7 |
| 04JAN17.D | Calibration | Fluorobenzene | 3.751 | 287653 | 836278 | 0.3440 | 258.9535 | 250.0000 | 103.6 |
| 04JAN19.D | Calibration | Fluorobenzene | 3.751 | 437439 | 841876 | 0.5196 | 391.1767 | 375.0000 | 104.3 |
| 04JAN21.D | Calibration | Fluorobenzene | 3.754 | 584294 | 841364 | 0.6945 | 522.8187 | 500.0000 | 104.6 |
| 04JAN23.D | QC | Fluorobenzene | 3.754 | 143378 | 801210 | 0.1790 | 134.7224 | 125.0000 | |

Compound: 1,1-Dichloroethane

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Fluorobenzene | | | 775552 | | ND | | |
| 04JAN10.D | Calibration | Fluorobenzene | 4.376 | 3892 | 770895 | 0.0050 | 2.6393 | 2.5000 | 105.6 |
| 04JAN11.D | Calibration | Fluorobenzene | 4.378 | 17642 | 764419 | 0.0231 | 12.0652 | 12.5000 | 96.5 |
| 04JAN12.D | Calibration | Fluorobenzene | 4.379 | 38874 | 791270 | 0.0491 | 25.6835 | 25.0000 | 102.7 |
| 04JAN13.D | Calibration | Fluorobenzene | 4.381 | 73205 | 778120 | 0.0941 | 49.1828 | 50.0000 | 98.4 |
| 04JAN15.D | Calibration | Fluorobenzene | 4.378 | 186052 | 823488 | 0.2259 | 118.1125 | 125.0000 | 94.5 |
| 04JAN17.D | Calibration | Fluorobenzene | 4.384 | 413408 | 836278 | 0.4943 | 258.4325 | 250.0000 | 103.4 |
| 04JAN19.D | Calibration | Fluorobenzene | 4.381 | 612660 | 841876 | 0.7277 | 380.4437 | 375.0000 | 101.5 |
| 04JAN21.D | Calibration | Fluorobenzene | 4.378 | 829359 | 841364 | 0.9857 | 515.3207 | 500.0000 | 103.1 |
| 04JAN23.D | QC | Fluorobenzene | 4.376 | 208131 | 801210 | 0.2598 | 135.8030 | 125.0000 | |

Compound: 2,2-Dichloropropane

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Fluorobenzene | | | 775552 | | ND | | |
| 04JAN10.D | Calibration | Fluorobenzene | 5.196 | 2930 | 770895 | 0.0038 | 2.6520 | 2.5000 | 106.1 |
| 04JAN11.D | Calibration | Fluorobenzene | 5.196 | 13676 | 764419 | 0.0179 | 12.4820 | 12.5000 | 99.9 |
| 04JAN12.D | Calibration | Fluorobenzene | 5.190 | 29793 | 791270 | 0.0377 | 26.2692 | 25.0000 | 105.1 |
| 04JAN13.D | Calibration | Fluorobenzene | 5.193 | 56189 | 778120 | 0.0722 | 50.3804 | 50.0000 | 100.8 |
| 04JAN15.D | Calibration | Fluorobenzene | 5.196 | 139656 | 823488 | 0.1696 | 118.3203 | 125.0000 | 94.7 |

Quantitative Analysis Results Summary Report

Compound: 2,2-Dichloropropane

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN17.D | Calibration | Fluorobenzene | 5.190 | 303307 | 836278 | 0.3627 | 253.0397 | 250.0000 | 101.2 |
| 04JAN19.D | Calibration | Fluorobenzene | 5.190 | 446282 | 841876 | 0.5301 | 369.8436 | 375.0000 | 98.6 |
| 04JAN21.D | Calibration | Fluorobenzene | 5.190 | 601823 | 841364 | 0.7153 | 499.0473 | 500.0000 | 99.8 |
| 04JAN23.D | QC | Fluorobenzene | 5.190 | 150902 | 801210 | 0.1883 | 131.4031 | 125.0000 | |

Compound: cis-1,2-Dichloroethene

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Fluorobenzene | | | 775552 | | ND | | |
| 04JAN10.D | Calibration | Fluorobenzene | 5.212 | 2376 | 770895 | 0.0031 | 2.9581 | 2.5000 | 118.3 |
| 04JAN11.D | Calibration | Fluorobenzene | 5.221 | 10008 | 764419 | 0.0131 | 12.5659 | 12.5000 | 100.5 |
| 04JAN12.D | Calibration | Fluorobenzene | 5.212 | 20252 | 791270 | 0.0256 | 24.5653 | 25.0000 | 98.3 |
| 04JAN13.D | Calibration | Fluorobenzene | 5.209 | 39251 | 778120 | 0.0504 | 48.4154 | 50.0000 | 96.8 |
| 04JAN15.D | Calibration | Fluorobenzene | 5.215 | 100057 | 823488 | 0.1215 | 116.6190 | 125.0000 | 93.3 |
| 04JAN17.D | Calibration | Fluorobenzene | 5.215 | 228170 | 836278 | 0.2728 | 261.8706 | 250.0000 | 104.7 |
| 04JAN19.D | Calibration | Fluorobenzene | 5.212 | 339211 | 841876 | 0.4029 | 386.7236 | 375.0000 | 103.1 |
| 04JAN21.D | Calibration | Fluorobenzene | 5.212 | 452377 | 841364 | 0.5377 | 516.0544 | 500.0000 | 103.2 |
| 04JAN23.D | QC | Fluorobenzene | 5.209 | 108623 | 801210 | 0.1356 | 130.1231 | 125.0000 | |

Compound: Methyl ethyl ketone

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Fluorobenzene | | | 775552 | | ND | | |
| 04JAN10.D | Calibration | Fluorobenzene | 5.302 | 3035 | 770895 | 0.0039 | 27.8967 | 25.0000 | 111.6 |
| 04JAN11.D | Calibration | Fluorobenzene | 5.288 | 13167 | 764419 | 0.0172 | 122.0520 | 125.0000 | 97.6 |
| 04JAN12.D | Calibration | Fluorobenzene | 5.282 | 26248 | 791270 | 0.0332 | 235.0504 | 250.0000 | 94.0 |
| 04JAN13.D | Calibration | Fluorobenzene | 5.285 | 52648 | 778120 | 0.0677 | 479.4296 | 500.0000 | 95.9 |
| 04JAN15.D | Calibration | Fluorobenzene | 5.282 | 134730 | 823488 | 0.1636 | 1159.3019 | 1250.0000 | 92.7 |
| 04JAN17.D | Calibration | Fluorobenzene | 5.279 | 317271 | 836278 | 0.3794 | 2688.2474 | 2500.0000 | 107.5 |
| 04JAN19.D | Calibration | Fluorobenzene | 5.279 | 470653 | 841876 | 0.5591 | 3961.3410 | 3750.0000 | 105.6 |
| 04JAN21.D | Calibration | Fluorobenzene | 5.279 | 632539 | 841364 | 0.7518 | 5327.1253 | 5000.0000 | 106.5 |
| 04JAN23.D | QC | Fluorobenzene | 5.282 | 135511 | 801210 | 0.1691 | 1198.4439 | 1250.0000 | |

Compound: Bromochloromethane

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Fluorobenzene | | | 775552 | | ND | | |
| 04JAN10.D | Calibration | Fluorobenzene | 5.522 | 807 | 770895 | 0.0010 | 2.4260 | 2.5000 | 97.0 |
| 04JAN11.D | Calibration | Fluorobenzene | 5.516 | 4275 | 764419 | 0.0056 | 12.9568 | 12.5000 | 103.7 |
| 04JAN12.D | Calibration | Fluorobenzene | 5.522 | 8688 | 791270 | 0.0110 | 25.4383 | 25.0000 | 101.8 |
| 04JAN13.D | Calibration | Fluorobenzene | 5.516 | 17338 | 778120 | 0.0223 | 51.6233 | 50.0000 | 103.2 |
| 04JAN15.D | Calibration | Fluorobenzene | 5.519 | 41966 | 823488 | 0.0510 | 118.0683 | 125.0000 | 94.5 |
| 04JAN17.D | Calibration | Fluorobenzene | 5.519 | 89178 | 836278 | 0.1066 | 247.0586 | 250.0000 | 98.8 |
| 04JAN19.D | Calibration | Fluorobenzene | 5.516 | 135103 | 841876 | 0.1605 | 371.8004 | 375.0000 | 99.1 |
| 04JAN21.D | Calibration | Fluorobenzene | 5.519 | 179618 | 841364 | 0.2135 | 494.6054 | 500.0000 | 98.9 |

Quantitative Analysis Results Summary Report

Compound: Bromochloromethane

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|-------|-----------|------------|------------|-----------|----------|
| 04JAN23.D | QC | Fluorobenzene | 5.513 | 42744 | 801210 | 0.0533 | 123.6009 | 125.0000 | |

Compound: Chloroform

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Fluorobenzene | | | 775552 | | ND | | |
| 04JAN10.D | Calibration | Fluorobenzene | 5.659 | 4248 | 770895 | 0.0055 | 2.8946 | 2.5000 | 115.8 |
| 04JAN11.D | Calibration | Fluorobenzene | 5.656 | 19015 | 764419 | 0.0249 | 13.0668 | 12.5000 | 104.5 |
| 04JAN12.D | Calibration | Fluorobenzene | 5.653 | 36413 | 791270 | 0.0460 | 24.1734 | 25.0000 | 96.7 |
| 04JAN13.D | Calibration | Fluorobenzene | 5.650 | 71403 | 778120 | 0.0918 | 48.2031 | 50.0000 | 96.4 |
| 04JAN15.D | Calibration | Fluorobenzene | 5.653 | 179640 | 823488 | 0.2181 | 114.5912 | 125.0000 | 91.7 |
| 04JAN17.D | Calibration | Fluorobenzene | 5.653 | 394946 | 836278 | 0.4723 | 248.0804 | 250.0000 | 99.2 |
| 04JAN19.D | Calibration | Fluorobenzene | 5.650 | 588080 | 841876 | 0.6985 | 366.9389 | 375.0000 | 97.9 |
| 04JAN21.D | Calibration | Fluorobenzene | 5.653 | 783422 | 841364 | 0.9311 | 489.1221 | 500.0000 | 97.8 |
| 04JAN23.D | QC | Fluorobenzene | 5.647 | 183676 | 801210 | 0.2292 | 120.4236 | 125.0000 | |

Compound: 1,1,1-Trichloroethane

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Fluorobenzene | | | 775552 | | ND | | |
| 04JAN10.D | Calibration | Fluorobenzene | 5.831 | 3510 | 770895 | 0.0046 | 2.5521 | 2.5000 | 102.1 |
| 04JAN11.D | Calibration | Fluorobenzene | 5.837 | 16623 | 764419 | 0.0217 | 12.1891 | 12.5000 | 97.5 |
| 04JAN12.D | Calibration | Fluorobenzene | 5.826 | 35547 | 791270 | 0.0449 | 25.1809 | 25.0000 | 100.7 |
| 04JAN13.D | Calibration | Fluorobenzene | 5.834 | 67007 | 778120 | 0.0861 | 48.2688 | 50.0000 | 96.5 |
| 04JAN15.D | Calibration | Fluorobenzene | 5.834 | 174206 | 823488 | 0.2115 | 118.5764 | 125.0000 | 94.9 |
| 04JAN17.D | Calibration | Fluorobenzene | 5.831 | 386005 | 836278 | 0.4616 | 258.7228 | 250.0000 | 103.5 |
| 04JAN19.D | Calibration | Fluorobenzene | 5.831 | 580748 | 841876 | 0.6898 | 386.6625 | 375.0000 | 103.1 |
| 04JAN21.D | Calibration | Fluorobenzene | 5.834 | 778785 | 841364 | 0.9256 | 518.8312 | 500.0000 | 103.8 |
| 04JAN23.D | QC | Fluorobenzene | 5.831 | 183324 | 801210 | 0.2288 | 128.2524 | 125.0000 | |

Compound: Dibromofluoromethane

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Fluorobenzene | 5.848 | 203459 | 775552 | 0.2623 | 278.4635 | | |
| 04JAN10.D | Calibration | Fluorobenzene | 5.851 | 2508 | 770895 | 0.0033 | 3.4533 | 2.5000 | 138.1 |
| 04JAN11.D | Calibration | Fluorobenzene | 5.845 | 9074 | 764419 | 0.0119 | 12.6000 | 12.5000 | 100.8 |
| 04JAN12.D | Calibration | Fluorobenzene | 5.845 | 19100 | 791270 | 0.0241 | 25.6219 | 25.0000 | 102.5 |
| 04JAN13.D | Calibration | Fluorobenzene | 5.848 | 35309 | 778120 | 0.0454 | 48.1661 | 50.0000 | 96.3 |
| 04JAN15.D | Calibration | Fluorobenzene | 5.845 | 89307 | 823488 | 0.1084 | 115.1146 | 125.0000 | 92.1 |
| 04JAN17.D | Calibration | Fluorobenzene | 5.845 | 204073 | 836278 | 0.2440 | 259.0223 | 250.0000 | 103.6 |
| 04JAN19.D | Calibration | Fluorobenzene | 5.848 | 305158 | 841876 | 0.3625 | 384.7503 | 375.0000 | 102.6 |
| 04JAN21.D | Calibration | Fluorobenzene | 5.845 | 404568 | 841364 | 0.4808 | 510.3991 | 500.0000 | 102.1 |
| 04JAN23.D | QC | Fluorobenzene | 5.848 | 204707 | 801210 | 0.2555 | 271.1994 | 250.0000 | |

Quantitative Analysis Results Summary Report

Compound: Carbon tetrachloride

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Fluorobenzene | | | 775552 | | ND | | |
| 04JAN10.D | Calibration | Fluorobenzene | 6.029 | 4342 | 770895 | 0.0056 | 3.2043 | 2.5000 | 128.2 |
| 04JAN11.D | Calibration | Fluorobenzene | 6.021 | 16466 | 764419 | 0.0215 | 12.2545 | 12.5000 | 98.0 |
| 04JAN12.D | Calibration | Fluorobenzene | 6.024 | 34462 | 791270 | 0.0436 | 24.7773 | 25.0000 | 99.1 |
| 04JAN13.D | Calibration | Fluorobenzene | 6.026 | 65313 | 778120 | 0.0839 | 47.7520 | 50.0000 | 95.5 |
| 04JAN15.D | Calibration | Fluorobenzene | 6.024 | 172928 | 823488 | 0.2100 | 119.4667 | 125.0000 | 95.6 |
| 04JAN17.D | Calibration | Fluorobenzene | 6.026 | 383485 | 836278 | 0.4586 | 260.8774 | 250.0000 | 104.4 |
| 04JAN19.D | Calibration | Fluorobenzene | 6.024 | 572545 | 841876 | 0.6801 | 386.9014 | 375.0000 | 103.2 |
| 04JAN21.D | Calibration | Fluorobenzene | 6.024 | 770907 | 841364 | 0.9163 | 521.2630 | 500.0000 | 104.3 |
| 04JAN23.D | QC | Fluorobenzene | 6.027 | 181384 | 801210 | 0.2264 | 128.7928 | 125.0000 | |

Compound: 1,1-Dichloropropene

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Fluorobenzene | | | 775552 | | ND | | |
| 04JAN10.D | Calibration | Fluorobenzene | 6.041 | 2830 | 770895 | 0.0037 | 2.4201 | 2.5000 | 96.8 |
| 04JAN11.D | Calibration | Fluorobenzene | 6.038 | 13149 | 764419 | 0.0172 | 11.3397 | 12.5000 | 90.7 |
| 04JAN12.D | Calibration | Fluorobenzene | 6.038 | 29241 | 791270 | 0.0370 | 24.3617 | 25.0000 | 97.4 |
| 04JAN13.D | Calibration | Fluorobenzene | 6.035 | 56376 | 778120 | 0.0725 | 47.7627 | 50.0000 | 95.5 |
| 04JAN15.D | Calibration | Fluorobenzene | 6.038 | 149649 | 823488 | 0.1817 | 119.8002 | 125.0000 | 95.8 |
| 04JAN17.D | Calibration | Fluorobenzene | 6.038 | 335741 | 836278 | 0.4015 | 264.6638 | 250.0000 | 105.9 |
| 04JAN19.D | Calibration | Fluorobenzene | 6.040 | 507157 | 841876 | 0.6024 | 397.1322 | 375.0000 | 105.9 |
| 04JAN21.D | Calibration | Fluorobenzene | 6.038 | 693669 | 841364 | 0.8245 | 543.5121 | 500.0000 | 108.7 |
| 04JAN23.D | QC | Fluorobenzene | 6.038 | 150930 | 801210 | 0.1884 | 124.1853 | 125.0000 | |

Compound: 1,2-Dichloroethane-d4

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Fluorobenzene | 6.233 | 88174 | 775552 | 0.1137 | 279.3964 | | |
| 04JAN10.D | Calibration | Fluorobenzene | 6.233 | 923 | 770895 | 0.0012 | 2.9438 | 2.5000 | 117.8 |
| 04JAN11.D | Calibration | Fluorobenzene | 6.227 | 3938 | 764419 | 0.0052 | 12.6600 | 12.5000 | 101.3 |
| 04JAN12.D | Calibration | Fluorobenzene | 6.236 | 8284 | 791270 | 0.0105 | 25.7280 | 25.0000 | 102.9 |
| 04JAN13.D | Calibration | Fluorobenzene | 6.233 | 15238 | 778120 | 0.0196 | 48.1252 | 50.0000 | 96.3 |
| 04JAN15.D | Calibration | Fluorobenzene | 6.233 | 39086 | 823488 | 0.0475 | 116.6420 | 125.0000 | 93.3 |
| 04JAN17.D | Calibration | Fluorobenzene | 6.236 | 87876 | 836278 | 0.1051 | 258.2324 | 250.0000 | 103.3 |
| 04JAN19.D | Calibration | Fluorobenzene | 6.233 | 129608 | 841876 | 0.1540 | 378.3335 | 375.0000 | 100.9 |
| 04JAN21.D | Calibration | Fluorobenzene | 6.233 | 174713 | 841364 | 0.2077 | 510.3080 | 500.0000 | 102.1 |
| 04JAN23.D | QC | Fluorobenzene | 6.230 | 91382 | 801210 | 0.1141 | 280.2886 | 250.0000 | |

Compound: Benzene

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|-------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Fluorobenzene | 6.266 | 381 | 775552 | 0.0005 | 0.1233 | | |
| 04JAN10.D | Calibration | Fluorobenzene | 6.278 | 8408 | 770895 | 0.0109 | 2.7393 | 2.5000 | 109.6 |
| 04JAN11.D | Calibration | Fluorobenzene | 6.278 | 37071 | 764419 | 0.0485 | 12.1801 | 12.5000 | 97.4 |

Quantitative Analysis Results Summary Report

Compound: Benzene

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|---------|-----------|------------|------------|-----------|----------|
| 04JAN12.D | Calibration | Fluorobenzene | 6.278 | 74956 | 791270 | 0.0947 | 23.7919 | 25.0000 | 95.2 |
| 04JAN13.D | Calibration | Fluorobenzene | 6.277 | 148727 | 778120 | 0.1911 | 48.0054 | 50.0000 | 96.0 |
| 04JAN15.D | Calibration | Fluorobenzene | 6.278 | 383469 | 823488 | 0.4657 | 116.9553 | 125.0000 | 93.6 |
| 04JAN17.D | Calibration | Fluorobenzene | 6.280 | 857534 | 836278 | 1.0254 | 257.5416 | 250.0000 | 103.0 |
| 04JAN19.D | Calibration | Fluorobenzene | 6.278 | 1293370 | 841876 | 1.5363 | 385.8526 | 375.0000 | 102.9 |
| 04JAN21.D | Calibration | Fluorobenzene | 6.280 | 1714050 | 841364 | 2.0372 | 511.6658 | 500.0000 | 102.3 |
| 04JAN23.D | QC | Fluorobenzene | 6.280 | 418900 | 801210 | 0.5228 | 131.3139 | 125.0000 | |

Compound: 1,2-Dichloroethane

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Fluorobenzene | | | 775552 | | ND | | |
| 04JAN10.D | Calibration | Fluorobenzene | 6.322 | 2415 | 770895 | 0.0031 | 2.9090 | 2.5000 | 116.4 |
| 04JAN11.D | Calibration | Fluorobenzene | 6.322 | 10202 | 764419 | 0.0133 | 12.3906 | 12.5000 | 99.1 |
| 04JAN12.D | Calibration | Fluorobenzene | 6.322 | 19996 | 791270 | 0.0253 | 23.4616 | 25.0000 | 93.8 |
| 04JAN13.D | Calibration | Fluorobenzene | 6.325 | 41058 | 778120 | 0.0528 | 48.9880 | 50.0000 | 98.0 |
| 04JAN15.D | Calibration | Fluorobenzene | 6.322 | 104855 | 823488 | 0.1273 | 118.2143 | 125.0000 | 94.6 |
| 04JAN17.D | Calibration | Fluorobenzene | 6.322 | 226964 | 836278 | 0.2714 | 251.9675 | 250.0000 | 100.8 |
| 04JAN19.D | Calibration | Fluorobenzene | 6.322 | 332775 | 841876 | 0.3953 | 366.9787 | 375.0000 | 97.9 |
| 04JAN21.D | Calibration | Fluorobenzene | 6.322 | 450739 | 841364 | 0.5357 | 497.3699 | 500.0000 | 99.5 |
| 04JAN23.D | QC | Fluorobenzene | 6.325 | 104249 | 801210 | 0.1301 | 120.7991 | 125.0000 | |

Compound: Trichloroethene

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Chlorobenzene-d5 | | | 301196 | | ND | | |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 7.033 | 2372 | 296081 | 0.0080 | 2.6564 | 2.5000 | 106.3 |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 7.025 | 10442 | 296554 | 0.0352 | 11.6753 | 12.5000 | 93.4 |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 7.028 | 21946 | 301338 | 0.0728 | 24.1484 | 25.0000 | 96.6 |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 7.030 | 42682 | 300356 | 0.1421 | 47.1189 | 50.0000 | 94.2 |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 7.030 | 114123 | 306491 | 0.3724 | 123.4646 | 125.0000 | 98.8 |
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 7.030 | 250285 | 316399 | 0.7910 | 262.2931 | 250.0000 | 104.9 |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 7.028 | 374370 | 314668 | 1.1897 | 394.4896 | 375.0000 | 105.2 |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 7.028 | 505400 | 313585 | 1.6117 | 534.4007 | 500.0000 | 106.9 |
| 04JAN23.D | QC | Chlorobenzene-d5 | 7.025 | 121734 | 307868 | 0.3954 | 131.1096 | 125.0000 | |

Compound: 1,2-Dichloropropane

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|-------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Chlorobenzene-d5 | | | 301196 | | ND | | |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 7.273 | 2148 | 296081 | 0.0073 | 2.7347 | 2.5000 | 109.4 |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 7.270 | 9488 | 296554 | 0.0320 | 12.0602 | 12.5000 | 96.5 |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 7.270 | 20077 | 301338 | 0.0666 | 25.1147 | 25.0000 | 100.5 |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 7.273 | 37870 | 300356 | 0.1261 | 47.5273 | 50.0000 | 95.1 |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 7.270 | 99187 | 306491 | 0.3236 | 121.9890 | 125.0000 | 97.6 |

Quantitative Analysis Results Summary Report

Compound: 1,2-Dichloropropane

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 7.270 | 213800 | 316399 | 0.6757 | 254.7161 | 250.0000 | 101.9 |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 7.270 | 324602 | 314668 | 1.0316 | 388.8502 | 375.0000 | 103.7 |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 7.270 | 436057 | 313585 | 1.3906 | 524.1695 | 500.0000 | 104.8 |
| 04JAN23.D | QC | Chlorobenzene-d5 | 7.270 | 102633 | 307868 | 0.3334 | 125.6626 | 125.0000 | |

Compound: Dibromomethane

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Chlorobenzene-d5 | | | 301196 | | ND | | |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 7.396 | 902 | 296081 | 0.0030 | 2.7162 | 2.5000 | 108.6 |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 7.399 | 4675 | 296554 | 0.0158 | 14.0619 | 12.5000 | 112.5 |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 7.393 | 8055 | 301338 | 0.0267 | 23.8439 | 25.0000 | 95.4 |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 7.396 | 15989 | 300356 | 0.0532 | 47.4844 | 50.0000 | 95.0 |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 7.399 | 40628 | 306491 | 0.1326 | 118.2425 | 125.0000 | 94.6 |
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 7.396 | 89483 | 316399 | 0.2828 | 252.2734 | 250.0000 | 100.9 |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 7.396 | 134282 | 314668 | 0.4267 | 380.6547 | 375.0000 | 101.5 |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 7.396 | 176038 | 313585 | 0.5614 | 500.7456 | 500.0000 | 100.1 |
| 04JAN23.D | QC | Chlorobenzene-d5 | 7.393 | 43248 | 307868 | 0.1405 | 125.3047 | 125.0000 | |

Compound: Bromodichloromethane

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Chlorobenzene-d5 | | | 301196 | | ND | | |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 7.597 | 2536 | 296081 | 0.0086 | 2.7684 | 2.5000 | 110.7 |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 7.585 | 11562 | 296554 | 0.0390 | 12.6014 | 12.5000 | 100.8 |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 7.583 | 22743 | 301338 | 0.0755 | 24.3940 | 25.0000 | 97.6 |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 7.585 | 43900 | 300356 | 0.1462 | 47.2409 | 50.0000 | 94.5 |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 7.585 | 115664 | 306491 | 0.3774 | 121.9749 | 125.0000 | 97.6 |
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 7.582 | 251805 | 316399 | 0.7958 | 257.2286 | 250.0000 | 102.9 |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 7.585 | 375983 | 314668 | 1.1949 | 386.1940 | 375.0000 | 103.0 |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 7.585 | 502929 | 313585 | 1.6038 | 518.3718 | 500.0000 | 103.7 |
| 04JAN23.D | QC | Chlorobenzene-d5 | 7.585 | 122757 | 307868 | 0.3987 | 128.8759 | 125.0000 | |

Compound: cis-1,3-Dichloropropene

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Chlorobenzene-d5 | | | 301196 | | ND | | |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 8.054 | 2583 | 296081 | 0.0087 | 2.4939 | 2.5000 | 99.8 |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 8.062 | 12525 | 296554 | 0.0422 | 12.0738 | 12.5000 | 96.6 |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 8.057 | 24511 | 301338 | 0.0813 | 23.2528 | 25.0000 | 93.0 |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 8.057 | 48886 | 300356 | 0.1628 | 46.5283 | 50.0000 | 93.1 |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 8.059 | 129419 | 306491 | 0.4223 | 120.7116 | 125.0000 | 96.6 |
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 8.057 | 293617 | 316399 | 0.9280 | 265.2863 | 250.0000 | 106.1 |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 8.057 | 441168 | 314668 | 1.4020 | 400.7930 | 375.0000 | 106.9 |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 8.059 | 591147 | 313585 | 1.8851 | 538.9008 | 500.0000 | 107.8 |

Quantitative Analysis Results Summary Report

Compound: cis-1,3-Dichloropropene

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN23.D | QC | Chlorobenzene-d5 | 8.054 | 130910 | 307868 | 0.4252 | 121.5561 | 125.0000 | |

Compound: Toluene-d8

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|---------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Chlorobenzene-d5 | 8.319 | 770154 | 301196 | 2.5570 | 265.3436 | | |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 8.322 | 7777 | 296081 | 0.0263 | 2.7257 | 2.5000 | 109.0 |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 8.322 | 32318 | 296554 | 0.1090 | 11.3089 | 12.5000 | 90.5 |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 8.319 | 67673 | 301338 | 0.2246 | 23.3046 | 25.0000 | 93.2 |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 8.319 | 136453 | 300356 | 0.4543 | 47.1441 | 50.0000 | 94.3 |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 8.319 | 358186 | 306491 | 1.1687 | 121.2749 | 125.0000 | 97.0 |
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 8.319 | 823306 | 316399 | 2.6021 | 270.0265 | 250.0000 | 108.0 |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 8.322 | 1229775 | 314668 | 3.9082 | 405.5583 | 375.0000 | 108.1 |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 8.319 | 1644540 | 313585 | 5.2443 | 544.2136 | 500.0000 | 108.8 |
| 04JAN23.D | QC | Chlorobenzene-d5 | 8.322 | 821531 | 307868 | 2.6685 | 276.9106 | 250.0000 | |

Compound: Toluene

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|---------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Chlorobenzene-d5 | | | 301196 | | ND | | |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 8.380 | 5039 | 296081 | 0.0170 | 2.6145 | 2.5000 | 104.6 |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 8.388 | 21794 | 296554 | 0.0735 | 11.2899 | 12.5000 | 90.3 |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 8.389 | 46355 | 301338 | 0.1538 | 23.6319 | 25.0000 | 94.5 |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 8.388 | 91915 | 300356 | 0.3060 | 47.0116 | 50.0000 | 94.0 |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 8.389 | 244712 | 306491 | 0.7984 | 122.6571 | 125.0000 | 98.1 |
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 8.386 | 541945 | 316399 | 1.7129 | 263.1330 | 250.0000 | 105.3 |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 8.388 | 813204 | 314668 | 2.5843 | 397.0106 | 375.0000 | 105.9 |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 8.389 | 1095161 | 313585 | 3.4924 | 536.5101 | 500.0000 | 107.3 |
| 04JAN23.D | QC | Chlorobenzene-d5 | 8.386 | 264584 | 307868 | 0.8594 | 132.0244 | 125.0000 | |

Compound: trans-1,3-Dichloropropene

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Chlorobenzene-d5 | | | 301196 | | ND | | |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 8.634 | 1470 | 296081 | 0.0050 | 1.9942 | 2.5000 | 79.8 |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 8.645 | 8683 | 296554 | 0.0293 | 11.7589 | 12.5000 | 94.1 |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 8.634 | 17850 | 301338 | 0.0592 | 23.7894 | 25.0000 | 95.2 |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 8.639 | 35179 | 300356 | 0.1171 | 47.0378 | 50.0000 | 94.1 |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 8.637 | 92719 | 306491 | 0.3025 | 121.4929 | 125.0000 | 97.2 |
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 8.639 | 207833 | 316399 | 0.6569 | 263.8027 | 250.0000 | 105.5 |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 8.639 | 315063 | 314668 | 1.0013 | 402.1098 | 375.0000 | 107.2 |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 8.637 | 416771 | 313585 | 1.3291 | 533.7551 | 500.0000 | 106.8 |
| 04JAN23.D | QC | Chlorobenzene-d5 | 8.637 | 98907 | 307868 | 0.3213 | 129.0216 | 125.0000 | |

Quantitative Analysis Results Summary Report

Compound: 1,1,2-Trichloroethane

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Chlorobenzene-d5 | | | 301196 | | ND | | |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 8.810 | 960 | 296081 | 0.0032 | 2.5012 | 2.5000 | 100.0 |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 8.824 | 5090 | 296554 | 0.0172 | 13.2340 | 12.5000 | 105.9 |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 8.815 | 10099 | 301338 | 0.0335 | 25.8400 | 25.0000 | 103.4 |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 8.815 | 18884 | 300356 | 0.0629 | 48.4759 | 50.0000 | 97.0 |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 8.818 | 46673 | 306491 | 0.1523 | 117.4130 | 125.0000 | 93.9 |
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 8.815 | 101888 | 316399 | 0.3220 | 248.2882 | 250.0000 | 99.3 |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 8.818 | 152331 | 314668 | 0.4841 | 373.2534 | 375.0000 | 99.5 |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 8.815 | 205463 | 313585 | 0.6552 | 505.1803 | 500.0000 | 101.0 |
| 04JAN23.D | QC | Chlorobenzene-d5 | 8.815 | 49128 | 307868 | 0.1596 | 123.0361 | 125.0000 | |

Compound: Tetrachloroethene

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Chlorobenzene-d5 | | | 301196 | | ND | | |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 8.932 | 2105 | 296081 | 0.0071 | 2.6772 | 2.5000 | 107.1 |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 8.935 | 9238 | 296554 | 0.0312 | 11.7302 | 12.5000 | 93.8 |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 8.935 | 20322 | 301338 | 0.0674 | 25.3948 | 25.0000 | 101.6 |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 8.935 | 36925 | 300356 | 0.1229 | 46.2932 | 50.0000 | 92.6 |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 8.935 | 97590 | 306491 | 0.3184 | 119.9003 | 125.0000 | 95.9 |
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 8.938 | 218245 | 316399 | 0.6898 | 259.7419 | 250.0000 | 103.9 |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 8.938 | 319950 | 314668 | 1.0168 | 382.8796 | 375.0000 | 102.1 |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 8.938 | 428812 | 313585 | 1.3675 | 514.9255 | 500.0000 | 103.0 |
| 04JAN23.D | QC | Chlorobenzene-d5 | 8.935 | 103027 | 307868 | 0.3346 | 126.0141 | 125.0000 | |

Compound: 1,3-Dichloropropane

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Chlorobenzene-d5 | | | 301196 | | ND | | |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 8.977 | 2257 | 296081 | 0.0076 | 2.9881 | 2.5000 | 119.5 |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 8.985 | 8967 | 296554 | 0.0302 | 11.8526 | 12.5000 | 94.8 |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 8.983 | 18745 | 301338 | 0.0622 | 24.3839 | 25.0000 | 97.5 |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 8.980 | 37457 | 300356 | 0.1247 | 48.8841 | 50.0000 | 97.8 |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 8.980 | 96183 | 306491 | 0.3138 | 123.0132 | 125.0000 | 98.4 |
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 8.980 | 212669 | 316399 | 0.6722 | 263.4754 | 250.0000 | 105.4 |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 8.980 | 312547 | 314668 | 0.9933 | 389.3442 | 375.0000 | 103.8 |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 8.980 | 408993 | 313585 | 1.3042 | 511.2479 | 500.0000 | 102.2 |
| 04JAN23.D | QC | Chlorobenzene-d5 | 8.980 | 95697 | 307868 | 0.3108 | 121.8442 | 125.0000 | |

Compound: Chlorodibromomethane

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Chlorobenzene-d5 | | | 301196 | | ND | | |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 9.203 | 1468 | 296081 | 0.0050 | 2.4461 | 2.5000 | 97.8 |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 9.206 | 7718 | 296554 | 0.0260 | 12.8393 | 12.5000 | 102.7 |

Quantitative Analysis Results Summary Report

Compound: Chlorodibromomethane

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 9.197 | 14873 | 301338 | 0.0494 | 24.3492 | 25.0000 | 97.4 |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 9.203 | 28153 | 300356 | 0.0937 | 46.2411 | 50.0000 | 92.5 |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 9.206 | 75015 | 306491 | 0.2448 | 120.7454 | 125.0000 | 96.6 |
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 9.203 | 165695 | 316399 | 0.5237 | 258.3535 | 250.0000 | 103.3 |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 9.203 | 247279 | 314668 | 0.7858 | 387.6812 | 375.0000 | 103.4 |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 9.203 | 330813 | 313585 | 1.0549 | 520.4361 | 500.0000 | 104.1 |
| 04JAN23.D | QC | Chlorobenzene-d5 | 9.203 | 78076 | 307868 | 0.2536 | 125.1103 | 125.0000 | |

Compound: 1,2-Dibromoethane

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Chlorobenzene-d5 | | | 301196 | | ND | | |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 9.300 | 1299 | 296081 | 0.0044 | 3.0943 | 2.5000 | 123.8 |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 9.300 | 5410 | 296554 | 0.0182 | 12.8640 | 12.5000 | 102.9 |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 9.309 | 10410 | 301338 | 0.0345 | 24.3601 | 25.0000 | 97.4 |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 9.303 | 21037 | 300356 | 0.0700 | 49.3889 | 50.0000 | 98.8 |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 9.306 | 51827 | 306491 | 0.1691 | 119.2394 | 125.0000 | 95.4 |
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 9.306 | 115714 | 316399 | 0.3657 | 257.8887 | 250.0000 | 103.2 |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 9.306 | 168577 | 314668 | 0.5357 | 377.7698 | 375.0000 | 100.7 |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 9.303 | 225877 | 313585 | 0.7203 | 507.9234 | 500.0000 | 101.6 |
| 04JAN23.D | QC | Chlorobenzene-d5 | 9.306 | 54259 | 307868 | 0.1762 | 124.2764 | 125.0000 | |

Compound: Chlorobenzene

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|---------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Chlorobenzene-d5 | | | 301196 | | ND | | |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 9.805 | 5771 | 296081 | 0.0195 | 2.7350 | 2.5000 | 109.4 |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 9.802 | 26461 | 296554 | 0.0892 | 12.5204 | 12.5000 | 100.2 |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 9.802 | 53047 | 301338 | 0.1760 | 24.7015 | 25.0000 | 98.8 |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 9.802 | 101452 | 300356 | 0.3378 | 47.3959 | 50.0000 | 94.8 |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 9.802 | 263617 | 306491 | 0.8601 | 120.6903 | 125.0000 | 96.6 |
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 9.802 | 582326 | 316399 | 1.8405 | 258.2544 | 250.0000 | 103.3 |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 9.802 | 867732 | 314668 | 2.7576 | 386.9455 | 375.0000 | 103.2 |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 9.802 | 1153147 | 313585 | 3.6773 | 515.9957 | 500.0000 | 103.2 |
| 04JAN23.D | QC | Chlorobenzene-d5 | 9.802 | 288815 | 307868 | 0.9381 | 131.6352 | 125.0000 | |

Compound: 1,1,1,2-Tetrachloroethane

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|-------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Chlorobenzene-d5 | | | 301196 | | ND | | |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 9.889 | 1893 | 296081 | 0.0064 | 2.5659 | 2.5000 | 102.6 |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 9.889 | 9473 | 296554 | 0.0319 | 12.8225 | 12.5000 | 102.6 |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 9.889 | 18130 | 301338 | 0.0602 | 24.1509 | 25.0000 | 96.6 |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 9.889 | 35544 | 300356 | 0.1183 | 47.5029 | 50.0000 | 95.0 |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 9.889 | 90898 | 306491 | 0.2966 | 119.0492 | 125.0000 | 95.2 |

Quantitative Analysis Results Summary Report

Compound: 1,1,1,2-Tetrachloroethane

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 9.891 | 200859 | 316399 | 0.6348 | 254.8274 | 250.0000 | 101.9 |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 9.892 | 307436 | 314668 | 0.9770 | 392.1859 | 375.0000 | 104.6 |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 9.892 | 406450 | 313585 | 1.2961 | 520.2855 | 500.0000 | 104.1 |
| 04JAN23.D | QC | Chlorobenzene-d5 | 9.892 | 97148 | 307868 | 0.3156 | 126.6657 | 125.0000 | |

Compound: Ethylbenzene

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|---------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Chlorobenzene-d5 | | | 301196 | | ND | | |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 9.920 | 9283 | 296081 | 0.0314 | 2.5367 | 2.5000 | 101.5 |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 9.917 | 40470 | 296554 | 0.1365 | 11.0411 | 12.5000 | 88.3 |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 9.917 | 88428 | 301338 | 0.2935 | 23.7421 | 25.0000 | 95.0 |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 9.917 | 173769 | 300356 | 0.5785 | 46.8079 | 50.0000 | 93.6 |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 9.920 | 464148 | 306491 | 1.5144 | 122.5243 | 125.0000 | 98.0 |
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 9.919 | 1043443 | 316399 | 3.2979 | 266.8193 | 250.0000 | 106.7 |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 9.919 | 1574219 | 314668 | 5.0028 | 404.7587 | 375.0000 | 107.9 |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 9.919 | 2111152 | 313585 | 6.7323 | 544.6881 | 500.0000 | 108.9 |
| 04JAN23.D | QC | Chlorobenzene-d5 | 9.917 | 501953 | 307868 | 1.6304 | 131.9113 | 125.0000 | |

Compound: m+p-Xylenes

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|--------|---------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Chlorobenzene-d5 | | | 301196 | | ND | | |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 10.045 | 7212 | 296081 | 0.0244 | 5.0712 | 5.0000 | 101.4 |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 10.037 | 31538 | 296554 | 0.1063 | 22.1410 | 25.0000 | 88.6 |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 10.039 | 66267 | 301338 | 0.2199 | 45.7836 | 50.0000 | 91.6 |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 10.039 | 133498 | 300356 | 0.4445 | 92.5347 | 100.0000 | 92.5 |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 10.039 | 368418 | 306491 | 1.2021 | 250.2587 | 250.0000 | 100.1 |
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 10.039 | 825866 | 316399 | 2.6102 | 543.4262 | 500.0000 | 108.7 |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 10.039 | 1228570 | 314668 | 3.9043 | 812.8556 | 750.0000 | 108.4 |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 10.039 | 1637879 | 313585 | 5.2231 | 1087.4082 | 1000.0000 | 108.7 |
| 04JAN23.D | QC | Chlorobenzene-d5 | 10.039 | 388558 | 307868 | 1.2621 | 262.7589 | 250.0000 | |

Compound: o-Xylene

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|--------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Chlorobenzene-d5 | | | 301196 | | ND | | |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 10.430 | 3330 | 296081 | 0.0112 | 2.6303 | 2.5000 | 105.2 |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 10.430 | 13519 | 296554 | 0.0456 | 10.6612 | 12.5000 | 85.3 |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 10.427 | 30463 | 301338 | 0.1011 | 23.6420 | 25.0000 | 94.6 |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 10.430 | 61016 | 300356 | 0.2031 | 47.5086 | 50.0000 | 95.0 |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 10.430 | 161509 | 306491 | 0.5270 | 123.2378 | 125.0000 | 98.6 |
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 10.430 | 365914 | 316399 | 1.1565 | 270.4636 | 250.0000 | 108.2 |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 10.433 | 549244 | 314668 | 1.7455 | 408.2043 | 375.0000 | 108.9 |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 10.430 | 734101 | 313585 | 2.3410 | 547.4764 | 500.0000 | 109.5 |

Quantitative Analysis Results Summary Report

Compound: o-Xylene

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|--------|--------|-----------|------------|------------|-----------|----------|
| 04JAN23.D | QC | Chlorobenzene-d5 | 10.430 | 174061 | 307868 | 0.5654 | 132.2214 | 125.0000 | |

Compound: Styrene

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|--------|---------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | Chlorobenzene-d5 | | | 301196 | | ND | | |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 10.444 | 4408 | 296081 | 0.0149 | 2.1625 | 2.5000 | 86.5 |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 10.449 | 23472 | 296554 | 0.0791 | 11.4968 | 12.5000 | 92.0 |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 10.447 | 48569 | 301338 | 0.1612 | 23.4119 | 25.0000 | 93.6 |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 10.444 | 96576 | 300356 | 0.3215 | 46.7052 | 50.0000 | 93.4 |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 10.447 | 268375 | 306491 | 0.8756 | 127.1910 | 125.0000 | 101.8 |
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 10.446 | 605646 | 316399 | 1.9142 | 278.0455 | 250.0000 | 111.2 |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 10.447 | 896331 | 314668 | 2.8485 | 413.7595 | 375.0000 | 110.3 |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 10.449 | 1199879 | 313585 | 3.8263 | 555.7946 | 500.0000 | 111.2 |
| 04JAN23.D | QC | Chlorobenzene-d5 | 10.449 | 291425 | 307868 | 0.9466 | 137.4974 | 125.0000 | |

Compound: Bromoform

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------------|--------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | 1,4-Dichlorobenzene-d4 | | | 231562 | | ND | | |
| 04JAN10.D | Calibration | 1,4-Dichlorobenzene-d4 | 10.625 | 708 | 227879 | 0.0031 | 2.4287 | 2.5000 | 97.1 |
| 04JAN11.D | Calibration | 1,4-Dichlorobenzene-d4 | 10.625 | 3652 | 242142 | 0.0151 | 11.7860 | 12.5000 | 94.3 |
| 04JAN12.D | Calibration | 1,4-Dichlorobenzene-d4 | 10.625 | 7972 | 240335 | 0.0332 | 25.9212 | 25.0000 | 103.7 |
| 04JAN13.D | Calibration | 1,4-Dichlorobenzene-d4 | 10.625 | 16073 | 248636 | 0.0646 | 50.5170 | 50.0000 | 101.0 |
| 04JAN15.D | Calibration | 1,4-Dichlorobenzene-d4 | 10.628 | 39165 | 264477 | 0.1481 | 115.7218 | 125.0000 | 92.6 |
| 04JAN17.D | Calibration | 1,4-Dichlorobenzene-d4 | 10.628 | 87836 | 266553 | 0.3295 | 257.5099 | 250.0000 | 103.0 |
| 04JAN19.D | Calibration | 1,4-Dichlorobenzene-d4 | 10.628 | 129038 | 266611 | 0.4840 | 378.2200 | 375.0000 | 100.9 |
| 04JAN21.D | Calibration | 1,4-Dichlorobenzene-d4 | 10.625 | 175918 | 262971 | 0.6690 | 522.7660 | 500.0000 | 104.6 |
| 04JAN23.D | QC | 1,4-Dichlorobenzene-d4 | 10.628 | 42560 | 255907 | 0.1663 | 129.9644 | 125.0000 | |

Compound: p-Bromofluorobenzene

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------------|--------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | 1,4-Dichlorobenzene-d4 | 10.951 | 226743 | 231562 | 0.9792 | 267.2815 | | |
| 04JAN10.D | Calibration | 1,4-Dichlorobenzene-d4 | 10.951 | 2719 | 227879 | 0.0119 | 3.2569 | 2.5000 | 130.3 |
| 04JAN11.D | Calibration | 1,4-Dichlorobenzene-d4 | 10.948 | 10059 | 242142 | 0.0415 | 11.3393 | 12.5000 | 90.7 |
| 04JAN12.D | Calibration | 1,4-Dichlorobenzene-d4 | 10.951 | 22267 | 240335 | 0.0926 | 25.2899 | 25.0000 | 101.2 |
| 04JAN13.D | Calibration | 1,4-Dichlorobenzene-d4 | 10.951 | 42506 | 248636 | 0.1710 | 46.6647 | 50.0000 | 93.3 |
| 04JAN15.D | Calibration | 1,4-Dichlorobenzene-d4 | 10.954 | 114269 | 264477 | 0.4321 | 117.9350 | 125.0000 | 94.3 |
| 04JAN17.D | Calibration | 1,4-Dichlorobenzene-d4 | 10.951 | 261042 | 266553 | 0.9793 | 267.3186 | 250.0000 | 106.9 |
| 04JAN19.D | Calibration | 1,4-Dichlorobenzene-d4 | 10.951 | 385474 | 266611 | 1.4458 | 394.6566 | 375.0000 | 105.2 |
| 04JAN21.D | Calibration | 1,4-Dichlorobenzene-d4 | 10.949 | 521580 | 262971 | 1.9834 | 541.3964 | 500.0000 | 108.3 |
| 04JAN23.D | QC | 1,4-Dichlorobenzene-d4 | 10.951 | 253034 | 255907 | 0.9888 | 269.8976 | 250.0000 | |

Quantitative Analysis Results Summary Report

Compound: Bromobenzene

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------------|--------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | 1,4-Dichlorobenzene-d4 | | | 231562 | | ND | | |
| 04JAN10.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.088 | 2024 | 227879 | 0.0089 | 2.7439 | 2.5000 | 109.8 |
| 04JAN11.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.096 | 9663 | 242142 | 0.0399 | 12.3310 | 12.5000 | 98.6 |
| 04JAN12.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.094 | 19259 | 240335 | 0.0801 | 24.7613 | 25.0000 | 99.0 |
| 04JAN13.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.093 | 38282 | 248636 | 0.1540 | 47.5759 | 50.0000 | 95.2 |
| 04JAN15.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.094 | 102265 | 264477 | 0.3867 | 119.4801 | 125.0000 | 95.6 |
| 04JAN17.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.093 | 227127 | 266553 | 0.8521 | 263.2944 | 250.0000 | 105.3 |
| 04JAN19.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.093 | 333431 | 266611 | 1.2506 | 386.4420 | 375.0000 | 103.1 |
| 04JAN21.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.094 | 439147 | 262971 | 1.6699 | 516.0104 | 500.0000 | 103.2 |
| 04JAN23.D | QC | 1,4-Dichlorobenzene-d4 | 11.093 | 109054 | 255907 | 0.4261 | 131.6788 | 125.0000 | |

Compound: 1,1,2,2-Tetrachloroethane

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------------|--------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | 1,4-Dichlorobenzene-d4 | | | 231562 | | ND | | |
| 04JAN10.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.113 | 1142 | 227879 | 0.0050 | 2.6916 | 2.5000 | 107.7 |
| 04JAN11.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.116 | 5793 | 242142 | 0.0239 | 12.8437 | 12.5000 | 102.7 |
| 04JAN12.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.110 | 12440 | 240335 | 0.0518 | 27.7883 | 25.0000 | 111.2 |
| 04JAN13.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.105 | 22514 | 248636 | 0.0906 | 48.6124 | 50.0000 | 97.2 |
| 04JAN15.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.116 | 56958 | 264477 | 0.2154 | 115.6179 | 125.0000 | 92.5 |
| 04JAN17.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.113 | 124205 | 266553 | 0.4660 | 250.1577 | 250.0000 | 100.1 |
| 04JAN19.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.110 | 182470 | 266611 | 0.6844 | 367.4276 | 375.0000 | 98.0 |
| 04JAN21.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.113 | 240837 | 262971 | 0.9158 | 491.6700 | 500.0000 | 98.3 |
| 04JAN23.D | QC | 1,4-Dichlorobenzene-d4 | 11.113 | 60763 | 255907 | 0.2374 | 127.4722 | 125.0000 | |

Compound: 1,2,3-Trichloropropane

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------------|--------|-------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | 1,4-Dichlorobenzene-d4 | | | 231562 | | ND | | |
| 04JAN10.D | Calibration | 1,4-Dichlorobenzene-d4 | | | 227879 | | ND | 2.5000 | |
| 04JAN11.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.144 | 1654 | 242142 | 0.0068 | 13.7084 | 12.5000 | 109.7 |
| 04JAN12.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.149 | 3200 | 240335 | 0.0133 | 26.7144 | 25.0000 | 106.9 |
| 04JAN13.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.146 | 6096 | 248636 | 0.0245 | 49.1924 | 50.0000 | 98.4 |
| 04JAN15.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.147 | 14846 | 264477 | 0.0561 | 112.6261 | 125.0000 | 90.1 |
| 04JAN17.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.152 | 33115 | 266553 | 0.1242 | 249.2635 | 250.0000 | 99.7 |
| 04JAN19.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.149 | 48325 | 266611 | 0.1813 | 363.6732 | 375.0000 | 97.0 |
| 04JAN21.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.146 | 64422 | 262971 | 0.2450 | 491.5229 | 500.0000 | 98.3 |
| 04JAN23.D | QC | 1,4-Dichlorobenzene-d4 | 11.146 | 15682 | 255907 | 0.0613 | 122.9523 | 125.0000 | |

Compound: 2-Chlorotoluene

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------------|--------|------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | 1,4-Dichlorobenzene-d4 | | | 231562 | | ND | | |
| 04JAN10.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.292 | 1844 | 227879 | 0.0081 | 2.5124 | 2.5000 | 100.5 |
| 04JAN11.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.289 | 8731 | 242142 | 0.0361 | 11.1977 | 12.5000 | 89.6 |

Quantitative Analysis Results Summary Report

Compound: 2-Chlorotoluene

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------------|--------|--------|-----------|------------|------------|-----------|----------|
| 04JAN12.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.286 | 19390 | 240335 | 0.0807 | 25.0550 | 25.0000 | 100.2 |
| 04JAN13.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.289 | 37987 | 248636 | 0.1528 | 47.4466 | 50.0000 | 94.9 |
| 04JAN15.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.292 | 102424 | 264477 | 0.3873 | 120.2675 | 125.0000 | 96.2 |
| 04JAN17.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.291 | 229396 | 266553 | 0.8606 | 267.2616 | 250.0000 | 106.9 |
| 04JAN19.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.291 | 336386 | 266611 | 1.2617 | 391.8269 | 375.0000 | 104.5 |
| 04JAN21.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.292 | 455991 | 262971 | 1.7340 | 538.4964 | 500.0000 | 107.7 |
| 04JAN23.D | QC | 1,4-Dichlorobenzene-d4 | 11.291 | 108192 | 255907 | 0.4228 | 131.2948 | 125.0000 | |

Compound: 4-Chlorotoluene

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------------|--------|---------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | 1,4-Dichlorobenzene-d4 | | | 231562 | | ND | | |
| 04JAN10.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.400 | 5419 | 227879 | 0.0238 | 2.2650 | 2.5000 | 90.6 |
| 04JAN11.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.400 | 28532 | 242142 | 0.1178 | 11.2233 | 12.5000 | 89.8 |
| 04JAN12.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.400 | 61551 | 240335 | 0.2561 | 24.3936 | 25.0000 | 97.6 |
| 04JAN13.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.400 | 126308 | 248636 | 0.5080 | 48.3865 | 50.0000 | 96.8 |
| 04JAN15.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.400 | 336146 | 264477 | 1.2710 | 121.0591 | 125.0000 | 96.8 |
| 04JAN17.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.400 | 748435 | 266553 | 2.8078 | 267.4409 | 250.0000 | 107.0 |
| 04JAN19.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.400 | 1109221 | 266611 | 4.1604 | 396.2756 | 375.0000 | 105.7 |
| 04JAN21.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.400 | 1468376 | 262971 | 5.5838 | 531.8471 | 500.0000 | 106.4 |
| 04JAN23.D | QC | 1,4-Dichlorobenzene-d4 | 11.400 | 368295 | 255907 | 1.4392 | 137.0790 | 125.0000 | |

Compound: 1,3-Dichlorobenzene

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------------|--------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | 1,4-Dichlorobenzene-d4 | | | 231562 | | ND | | |
| 04JAN10.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.033 | 3541 | 227879 | 0.0155 | 2.6327 | 2.5000 | 105.3 |
| 04JAN11.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.036 | 16932 | 242142 | 0.0699 | 11.8473 | 12.5000 | 94.8 |
| 04JAN12.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.033 | 36559 | 240335 | 0.1521 | 25.7725 | 25.0000 | 103.1 |
| 04JAN13.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.033 | 69539 | 248636 | 0.2797 | 47.3853 | 50.0000 | 94.8 |
| 04JAN15.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.031 | 183404 | 264477 | 0.6935 | 117.4899 | 125.0000 | 94.0 |
| 04JAN17.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.033 | 406895 | 266553 | 1.5265 | 258.6297 | 250.0000 | 103.5 |
| 04JAN19.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.033 | 603674 | 266611 | 2.2643 | 383.6225 | 375.0000 | 102.3 |
| 04JAN21.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.033 | 793993 | 262971 | 3.0193 | 511.5504 | 500.0000 | 102.3 |
| 04JAN23.D | QC | 1,4-Dichlorobenzene-d4 | 12.033 | 204088 | 255907 | 0.7975 | 135.1185 | 125.0000 | |

Compound: 1,4-Dichlorobenzene

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------------|--------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | 1,4-Dichlorobenzene-d4 | | | 231562 | | ND | | |
| 04JAN10.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.125 | 3787 | 227879 | 0.0166 | 2.7613 | 2.5000 | 110.5 |
| 04JAN11.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.122 | 17438 | 242142 | 0.0720 | 11.9662 | 12.5000 | 95.7 |
| 04JAN12.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.125 | 36635 | 240335 | 0.1524 | 25.3284 | 25.0000 | 101.3 |
| 04JAN13.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.125 | 71841 | 248636 | 0.2889 | 48.0106 | 50.0000 | 96.0 |
| 04JAN15.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.125 | 189045 | 264477 | 0.7148 | 118.7699 | 125.0000 | 95.0 |

Quantitative Analysis Results Summary Report

Compound: 1,4-Dichlorobenzene

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------------|--------|--------|-----------|------------|------------|-----------|----------|
| 04JAN17.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.122 | 408934 | 266553 | 1.5342 | 254.9170 | 250.0000 | 102.0 |
| 04JAN19.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.125 | 595919 | 266611 | 2.2352 | 371.3969 | 375.0000 | 99.0 |
| 04JAN21.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.125 | 794954 | 262971 | 3.0230 | 502.3001 | 500.0000 | 100.5 |
| 04JAN23.D | QC | 1,4-Dichlorobenzene-d4 | 12.122 | 200032 | 255907 | 0.7817 | 129.8812 | 125.0000 | |

Compound: 1,2-Dichlorobenzene

| Data File | Sample Type | ISTD | RT | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------------|--------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank | 1,4-Dichlorobenzene-d4 | | | 231562 | | ND | | |
| 04JAN10.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.499 | 3104 | 227879 | 0.0136 | 2.7307 | 2.5000 | 109.2 |
| 04JAN11.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.493 | 14666 | 242142 | 0.0606 | 12.1423 | 12.5000 | 97.1 |
| 04JAN12.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.488 | 29899 | 240335 | 0.1244 | 24.9402 | 25.0000 | 99.8 |
| 04JAN13.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.491 | 60213 | 248636 | 0.2422 | 48.5498 | 50.0000 | 97.1 |
| 04JAN15.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.493 | 152284 | 264477 | 0.5758 | 115.4323 | 125.0000 | 92.3 |
| 04JAN17.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.493 | 342576 | 266553 | 1.2852 | 257.6524 | 250.0000 | 103.1 |
| 04JAN19.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.493 | 499147 | 266611 | 1.8722 | 375.3283 | 375.0000 | 100.1 |
| 04JAN21.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.493 | 664247 | 262971 | 2.5259 | 506.3871 | 500.0000 | 101.3 |
| 04JAN23.D | QC | 1,4-Dichlorobenzene-d4 | 12.493 | 164299 | 255907 | 0.6420 | 128.7104 | 125.0000 | |

Initial Calibration Report - VOA5975C

Method Path \\MASSHUNTER\Org\Data\Methods\Quant\VOA5975C\VOA5975C_010422_CAL
 Method File VOA5975C_8260B_SHT_DoD_L4_010422.m
 Batch Name D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin
 Last Calib Update 1/9/2022 8:59:52 PM

| Level Name | Calibration Files | Acq. Date-Time | Level Last Update Time |
|------------|---|---------------------|------------------------|
| 1 | D:\Org\Data\VOA5975C\VG010422\04JAN10.D | 1/4/2022 3:33:04 PM | 1/5/2022 11:05:51 AM |
| 2 | D:\Org\Data\VOA5975C\VG010422\04JAN11.D | 1/4/2022 4:00:35 PM | 1/5/2022 11:05:51 AM |
| 3 | D:\Org\Data\VOA5975C\VG010422\04JAN12.D | 1/4/2022 4:28:05 PM | 1/5/2022 11:05:51 AM |
| 4 | D:\Org\Data\VOA5975C\VG010422\04JAN13.D | 1/4/2022 4:55:32 PM | 1/5/2022 11:05:51 AM |
| 5 | D:\Org\Data\VOA5975C\VG010422\04JAN15.D | 1/4/2022 5:50:25 PM | 1/5/2022 11:05:51 AM |
| 6 | D:\Org\Data\VOA5975C\VG010422\04JAN17.D | 1/4/2022 6:45:10 PM | 1/5/2022 11:05:51 AM |
| 7 | D:\Org\Data\VOA5975C\VG010422\04JAN19.D | 1/4/2022 7:39:45 PM | 1/5/2022 11:05:51 AM |
| 8 | D:\Org\Data\VOA5975C\VG010422\04JAN21.D | 1/4/2022 8:34:31 PM | 1/5/2022 11:05:51 AM |

| Compound | Curve Fit | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | Avg RF | %RSD |
|----------------------------------|-----------|--------|--------|--------|--------|--------|--------|--------|--------|----------|--------|
| ----- ISTD ----- | | | | | | | | | | | |
| I Fluorobenzene | | | | | | | | | | | |
| T Dichlorodifluoromethane | Avg RF | | 0.3162 | 0.3365 | 0.3242 | 0.3350 | 0.3304 | 0.3267 | 0.3242 | 0.3276 | 2.141 |
| T Chloromethane | Avg RF | | 0.4411 | 0.4190 | 0.3960 | 0.3901 | 0.3821 | 0.3733 | 0.3819 | 0.3976 | 6.061 |
| T Vinyl chloride | Avg RF | | 0.3591 | 0.3671 | 0.3503 | 0.3603 | 0.3559 | 0.3553 | 0.3566 | 0.3578 | 1.449 |
| T Bromomethane | Avg RF | | 0.1542 | 0.1650 | 0.1523 | 0.1583 | 0.1611 | 0.1643 | 0.1648 | 0.1600 | 3.267 |
| T Chloroethane | Avg RF | | 0.2107 | 0.1851 | 0.1638 | 0.1735 | 0.1642 | 0.1721 | 0.1706 | 0.1771 | 9.265 |
| T Trichlorofluoromethane | Avg RF | | 0.4037 | 0.4735 | 0.4380 | 0.4586 | 0.4602 | 0.4399 | 0.4349 | 0.4441 | 5.118 |
| T 1,1-Dichloroethene | Avg RF | | 0.2399 | 0.2607 | 0.2458 | 0.2415 | 0.2600 | 0.2554 | 0.2594 | 0.2518 | 3.629 |
| T Methylene chloride | Avg RF | | 0.4640 | 0.3906 | 0.3745 | 0.3285 | 0.3496 | 0.3446 | 0.3467 | 0.3712 | 12.340 |
| T trans-1,2-Dichloroethene | Avg RF | | 0.2570 | 0.2617 | 0.2544 | 0.2439 | 0.2617 | 0.2577 | 0.2621 | 0.2569 | 2.508 |
| T Methyl tert-butyl ether (MTBE) | Avg RF | | 0.3274 | 0.3061 | 0.3157 | 0.3378 | 0.3440 | 0.3464 | 0.3472 | 0.3321 | 4.880 |
| T 1,1-Dichloroethane | Avg RF | | 0.4616 | 0.4913 | 0.4704 | 0.4519 | 0.4943 | 0.4852 | 0.4929 | 0.4782 | 3.547 |
| T 2,2-Dichloropropane | Avg RF | | 0.3578 | 0.3765 | 0.3611 | 0.3392 | 0.3627 | 0.3534 | 0.3576 | 0.3583 | 3.118 |
| T cis-1,2-Dichloroethene | Avg RF | | 0.2618 | 0.2559 | 0.2522 | 0.2430 | 0.2728 | 0.2686 | 0.2688 | 0.2605 | 4.101 |
| T Methyl ethyl ketone | Avg RF | | 0.0344 | 0.0332 | 0.0338 | 0.0327 | 0.0379 | 0.0373 | 0.0376 | 0.0353 # | 6.353 |
| T Bromochloromethane | Avg RF | | 0.1118 | 0.1098 | 0.1114 | 0.1019 | 0.1066 | 0.1070 | 0.1067 | 0.1079 | 3.188 |
| T Chloroform | Avg RF | 0.5510 | 0.4975 | 0.4602 | 0.4588 | 0.4363 | 0.4723 | 0.4657 | 0.4656 | 0.4759 | 7.299 |
| T 1,1,1-Trichloroethane | Avg RF | | 0.4349 | 0.4492 | 0.4306 | 0.4231 | 0.4616 | 0.4599 | 0.4628 | 0.4460 | 3.677 |
| S Dibromofluoromethane | Avg RF | | 0.2374 | 0.2414 | 0.2269 | 0.2169 | 0.2440 | 0.2416 | 0.2404 | 0.2355 | 4.222 |
| T Carbon tetrachloride | Avg RF | | 0.4308 | 0.4355 | 0.4197 | 0.4200 | 0.4586 | 0.4534 | 0.4581 | 0.4394 | 3.906 |
| T 1,1-Dichloropropene | Avg RF | | 0.3440 | 0.3695 | 0.3623 | 0.3635 | 0.4015 | 0.4016 | 0.4122 | 0.3792 | 6.770 |
| S 1,2-Dichloroethane-d4 | Avg RF | | 0.1030 | 0.1047 | 0.0979 | 0.0949 | 0.1051 | 0.1026 | 0.1038 | 0.1017 | 3.759 |
| T Benzene | Avg RF | 1.0907 | 0.9699 | 0.9473 | 0.9557 | 0.9313 | 1.0254 | 1.0242 | 1.0186 | 0.9954 | 5.369 |
| T 1,2-Dichloroethane | Avg RF | 0.3133 | 0.2669 | 0.2527 | 0.2638 | 0.2547 | 0.2714 | 0.2635 | 0.2679 | 0.2693 | 7.024 |
| ----- ISTD ----- | | | | | | | | | | | |
| I Chlorobenzene-d5 | | | | | | | | | | | |
| T Trichloroethene | Avg RF | | 0.7042 | 0.7283 | 0.7105 | 0.7447 | 0.7910 | 0.7932 | 0.8058 | 0.7540 | 5.603 |
| T 1,2-Dichloropropane | Avg RF | | 0.6399 | 0.6663 | 0.6304 | 0.6472 | 0.6757 | 0.6877 | 0.6953 | 0.6632 | 3.729 |
| T Dibromomethane | Avg RF | | 0.3153 | 0.2673 | 0.2662 | 0.2651 | 0.2828 | 0.2845 | 0.2807 | 0.2803 | 6.261 |
| T Bromodichloromethane | Avg RF | | 0.7798 | 0.7547 | 0.7308 | 0.7548 | 0.7958 | 0.7966 | 0.8019 | 0.7735 | 3.503 |

Initial Calibration Report - VOA5975C

| Compound | Curve Fit | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | Avg RF | %RSD |
|-----------------------------|-----------|--------|--------|--------|--------|--------|--------|--------|--------|--------|-------|
| T cis-1,3-Dichloropropene | Avg RF | | 0.8447 | 0.8134 | 0.8138 | 0.8445 | 0.9280 | 0.9347 | 0.9426 | 0.8745 | 6.654 |
| S Toluene-d8 | Avg RF | | 2.1796 | 2.2458 | 2.2715 | 2.3373 | 2.6021 | 2.6054 | 2.6222 | 2.4091 | 8.032 |
| T Toluene | Avg RF | 1.7019 | 1.4698 | 1.5383 | 1.5301 | 1.5969 | 1.7129 | 1.7229 | 1.7462 | 1.6274 | 6.538 |
| T trans-1,3-Dichloropropene | Avg RF | | 0.5856 | 0.5924 | 0.5856 | 0.6050 | 0.6569 | 0.6675 | 0.6645 | 0.6225 | 6.190 |
| T 1,1,2-Trichloroethane | Avg RF | | 0.3433 | 0.3351 | 0.3144 | 0.3046 | 0.3220 | 0.3227 | 0.3276 | 0.3242 | 3.951 |
| T Tetrachloroethene | Avg RF | 0.7110 | 0.6230 | 0.6744 | 0.6147 | 0.6368 | 0.6898 | 0.6779 | 0.6837 | 0.6639 | 5.221 |
| T 1,3-Dichloropropane | Avg RF | | 0.6047 | 0.6221 | 0.6235 | 0.6276 | 0.6722 | 0.6622 | 0.6521 | 0.6378 | 3.855 |
| T Chlorodibromomethane | Avg RF | | 0.5205 | 0.4936 | 0.4687 | 0.4895 | 0.5237 | 0.5239 | 0.5275 | 0.5068 | 4.501 |
| T 1,2-Dibromoethane | Avg RF | | 0.3649 | 0.3455 | 0.3502 | 0.3382 | 0.3657 | 0.3572 | 0.3602 | 0.3545 | 2.909 |
| T Chlorobenzene | Avg RF | | 1.7846 | 1.7604 | 1.6889 | 1.7202 | 1.8405 | 1.8384 | 1.8387 | 1.7817 | 3.458 |
| T 1,1,1,2-Tetrachloroethane | Avg RF | | 0.6389 | 0.6016 | 0.5917 | 0.5932 | 0.6348 | 0.6513 | 0.6481 | 0.6228 | 4.223 |
| T Ethylbenzene | Avg RF | 3.1353 | 2.7294 | 2.9345 | 2.8927 | 3.0288 | 3.2979 | 3.3352 | 3.3662 | 3.0900 | 7.526 |
| T m+p-Xylenes | Avg RF | 1.2179 | 1.0635 | 1.0995 | 1.1112 | 1.2021 | 1.3051 | 1.3014 | 1.3058 | 1.2008 | 8.296 |
| T o-Xylene | Avg RF | | 0.9117 | 1.0109 | 1.0157 | 1.0539 | 1.1565 | 1.1636 | 1.1705 | 1.0690 | 9.204 |
| T Styrene | Avg RF | 1.4888 | 1.5830 | 1.6118 | 1.6077 | 1.7513 | 1.9142 | 1.8990 | 1.9132 | 1.7211 | 9.933 |
| I 1,4-Dichlorobenzene-d4 | | | | | | | | | | | |
| ----- ISTD ----- | | | | | | | | | | | |
| T Bromoform | Avg RF | | 0.3016 | 0.3317 | 0.3232 | 0.2962 | 0.3295 | 0.3227 | 0.3345 | 0.3199 | 4.706 |
| S p-Bromofluorobenzene | Avg RF | | 0.8308 | 0.9265 | 0.8548 | 0.8641 | 0.9793 | 0.9639 | 0.9917 | 0.9159 | 7.165 |
| T Bromobenzene | Avg RF | | 0.7981 | 0.8013 | 0.7698 | 0.7733 | 0.8521 | 0.8338 | 0.8350 | 0.8091 | 3.949 |
| T 1,1,2,2-Tetrachloroethane | Avg RF | | 0.4785 | 0.5176 | 0.4528 | 0.4307 | 0.4660 | 0.4563 | 0.4579 | 0.4657 | 5.814 |
| T 1,2,3-Trichloropropane | Avg RF | | 0.1366 | 0.1331 | 0.1226 | 0.1123 | 0.1242 | 0.1208 | 0.1225 | 0.1246 | 6.496 |
| T 2-Chlorotoluene | Avg RF | | 0.7211 | 0.8068 | 0.7639 | 0.7745 | 0.8606 | 0.8411 | 0.8670 | 0.8050 | 6.783 |
| T 4-Chlorotoluene | Avg RF | | 2.3566 | 2.5611 | 2.5400 | 2.5420 | 2.8078 | 2.7736 | 2.7919 | 2.6247 | 6.481 |
| T 1,3-Dichlorobenzene | Avg RF | 1.5539 | 1.3985 | 1.5212 | 1.3984 | 1.3869 | 1.5265 | 1.5095 | 1.5097 | 1.4756 | 4.644 |
| T 1,4-Dichlorobenzene | Avg RF | 1.6618 | 1.4403 | 1.5243 | 1.4447 | 1.4296 | 1.5342 | 1.4901 | 1.5115 | 1.5046 | 4.999 |
| T 1,2-Dichlorobenzene | Avg RF | 1.3621 | 1.2114 | 1.2441 | 1.2109 | 1.1516 | 1.2852 | 1.2481 | 1.2630 | 1.2470 | 4.949 |


(RedFont and #) = Outlier Flag; (I) = Internal Standard; (T) = Target; (S) = Surrogate; (M) = Matrix Spike

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:39 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

Dichlorodifluoromethane %RSE = 2.1

Dichlorodifluoromethane - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 4353 | 2.5000 | 0.5647 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 12087 | 12.5000 | 0.3162 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 26627 | 25.0000 | 0.3365 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 50457 | 50.0000 | 0.3242 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 116936 | 125.0000 | 0.2919 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 137933 | 125.0000 | 0.3350 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 137933 | 125.0000 | 0.3350 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 276334 | 250.0000 | 0.3304 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 412544 | 375.0000 | 0.3267 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 545484 | 500.0000 | 0.3242 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:42 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

Chloromethane %RSE = 6.1

Chloromethane - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 7435 | 2.5000 | 0.9645 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 16859 | 12.5000 | 0.4411 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 33153 | 25.0000 | 0.4190 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 61632 | 50.0000 | 0.3960 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 138617 | 125.0000 | 0.3460 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 160604 | 125.0000 | 0.3901 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 160604 | 125.0000 | 0.3901 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 319523 | 250.0000 | 0.3821 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 471454 | 375.0000 | 0.3733 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 642582 | 500.0000 | 0.3819 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:42 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

Vinyl chloride %RSE = 1.4

Vinyl chloride - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 4274 | 2.5000 | 0.5544 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 13724 | 12.5000 | 0.3591 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 29046 | 25.0000 | 0.3671 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 54521 | 50.0000 | 0.3503 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 137775 | 125.0000 | 0.3439 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 148358 | 125.0000 | 0.3603 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 148358 | 125.0000 | 0.3603 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 297604 | 250.0000 | 0.3559 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 448643 | 375.0000 | 0.3553 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 600092 | 500.0000 | 0.3566 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:42 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

Bromomethane %RSE = 3.3

Bromomethane - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 1902 | 2.5000 | 0.2467 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 5893 | 12.5000 | 0.1542 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 13054 | 25.0000 | 0.1650 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 23699 | 50.0000 | 0.1523 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 59947 | 125.0000 | 0.1496 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 65163 | 125.0000 | 0.1583 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 65163 | 125.0000 | 0.1583 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 134737 | 250.0000 | 0.1611 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 207491 | 375.0000 | 0.1643 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 277301 | 500.0000 | 0.1648 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:42 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

Chloroethane %RSE = 9.3

Chloroethane - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 2178 | 2.5000 | 0.2825 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 8052 | 12.5000 | 0.2107 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 14646 | 25.0000 | 0.1851 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 25484 | 50.0000 | 0.1638 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 65619 | 125.0000 | 0.1638 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 71420 | 125.0000 | 0.1735 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 71420 | 125.0000 | 0.1735 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 137312 | 250.0000 | 0.1642 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 217393 | 375.0000 | 0.1721 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 287041 | 500.0000 | 0.1706 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:43 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

Trichlorofluoromethane %RSE = 5.1

Trichlorofluoromethane - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 5030 | 2.5000 | 0.6525 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 15431 | 12.5000 | 0.4037 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 37464 | 25.0000 | 0.4735 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 68163 | 50.0000 | 0.4380 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 173333 | 125.0000 | 0.4327 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 188808 | 125.0000 | 0.4586 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 188808 | 125.0000 | 0.4586 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 384837 | 250.0000 | 0.4602 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 555477 | 375.0000 | 0.4399 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 731829 | 500.0000 | 0.4349 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:43 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

1,1-Dichloroethene %RSE = 3.6




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 2084 | 2.5000 | 0.2703 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 9169 | 12.5000 | 0.2399 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 20631 | 25.0000 | 0.2607 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 38253 | 50.0000 | 0.2458 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 108512 | 125.0000 | 0.2709 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 99438 | 125.0000 | 0.2415 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 99438 | 125.0000 | 0.2415 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 217406 | 250.0000 | 0.2600 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 322557 | 375.0000 | 0.2554 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 436507 | 500.0000 | 0.2594 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:43 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

Methylene chloride %RSE = 12.3




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 4095 | 2.5000 | 0.5312 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 17734 | 12.5000 | 0.4640 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 30908 | 25.0000 | 0.3906 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 58282 | 50.0000 | 0.3745 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 144585 | 125.0000 | 0.3609 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 135271 | 125.0000 | 0.3285 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 135271 | 125.0000 | 0.3285 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 292397 | 250.0000 | 0.3496 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 435116 | 375.0000 | 0.3446 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 583438 | 500.0000 | 0.3467 | |

Calibration Report

| | | | |
|---------------------|---|----------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:43 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

trans-1,2-Dichloroethene %RSE = 2.5

trans-1,2-Dichloroethene - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 2146 | 2.5000 | 0.2784 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 9821 | 12.5000 | 0.2570 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 20706 | 25.0000 | 0.2617 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 39596 | 50.0000 | 0.2544 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 110909 | 125.0000 | 0.2769 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 100409 | 125.0000 | 0.2439 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 100409 | 125.0000 | 0.2439 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 218855 | 250.0000 | 0.2617 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 325415 | 375.0000 | 0.2577 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 440967 | 500.0000 | 0.2621 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:43 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

Methyl tert-butyl ether (MTBE) %RSE = 4.9

Methyl tert-butyl ether (MTBE) - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 2717 | 2.5000 | 0.3524 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 12515 | 12.5000 | 0.3274 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 24218 | 25.0000 | 0.3061 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 49126 | 50.0000 | 0.3157 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 143378 | 125.0000 | 0.3579 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 139068 | 125.0000 | 0.3378 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 139068 | 125.0000 | 0.3378 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 287653 | 250.0000 | 0.3440 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 437439 | 375.0000 | 0.3464 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 584294 | 500.0000 | 0.3472 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:43 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

1,1-Dichloroethane %RSE = 3.5




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 3892 | 2.5000 | 0.5049 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 17642 | 12.5000 | 0.4616 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 38874 | 25.0000 | 0.4913 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 73205 | 50.0000 | 0.4704 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 208131 | 125.0000 | 0.5195 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 186052 | 125.0000 | 0.4519 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 186052 | 125.0000 | 0.4519 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 413408 | 250.0000 | 0.4943 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 612660 | 375.0000 | 0.4852 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 829359 | 500.0000 | 0.4929 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:43 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

2,2-Dichloropropane %RSE = 3.1

2,2-Dichloropropane - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 2930 | 2.5000 | 0.3801 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 13676 | 12.5000 | 0.3578 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 29793 | 25.0000 | 0.3765 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 56189 | 50.0000 | 0.3611 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 150902 | 125.0000 | 0.3767 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 139656 | 125.0000 | 0.3392 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 139656 | 125.0000 | 0.3392 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 303307 | 250.0000 | 0.3627 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 446282 | 375.0000 | 0.3534 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 601823 | 500.0000 | 0.3576 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:43 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

cis-1,2-Dichloroethene %RSE = 4.1

cis-1,2-Dichloroethene - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 2376 | 2.5000 | 0.3082 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 10008 | 12.5000 | 0.2618 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 20252 | 25.0000 | 0.2559 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 39251 | 50.0000 | 0.2522 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 108623 | 125.0000 | 0.2711 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 100057 | 125.0000 | 0.2430 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 100057 | 125.0000 | 0.2430 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 228170 | 250.0000 | 0.2728 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 339211 | 375.0000 | 0.2686 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 452377 | 500.0000 | 0.2688 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:43 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

Methyl ethyl ketone %RSE = 6.4




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 3035 | 25.0000 | 0.0394 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 13167 | 125.0000 | 0.0344 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 26248 | 250.0000 | 0.0332 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 52648 | 500.0000 | 0.0338 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 135511 | 1250.0000 | 0.0338 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 134730 | 1250.0000 | 0.0327 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 134730 | 1250.0000 | 0.0327 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 317271 | 2500.0000 | 0.0379 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 470653 | 3750.0000 | 0.0373 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 632539 | 5000.0000 | 0.0376 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:43 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

Bromochloromethane %RSE = 3.2

Bromochloromethane - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 807 | 2.5000 | 0.1047 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 4275 | 12.5000 | 0.1118 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 8688 | 25.0000 | 0.1098 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 17338 | 50.0000 | 0.1114 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 42744 | 125.0000 | 0.1067 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 41966 | 125.0000 | 0.1019 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 41966 | 125.0000 | 0.1019 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 89178 | 250.0000 | 0.1066 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 135103 | 375.0000 | 0.1070 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 179618 | 500.0000 | 0.1067 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:43 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

Chloroform %RSE = 7.3

Chloroform - 8 Levels, 8 Levels Used, 8 Points, 8 Points Used, 1 QCs




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | x | 4248 | 2.5000 | 0.5510 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 19015 | 12.5000 | 0.4975 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 36413 | 25.0000 | 0.4602 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 71403 | 50.0000 | 0.4588 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 183676 | 125.0000 | 0.4585 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 179640 | 125.0000 | 0.4363 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 179640 | 125.0000 | 0.4363 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 394946 | 250.0000 | 0.4723 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 588080 | 375.0000 | 0.4657 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 783422 | 500.0000 | 0.4656 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:43 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

1,1,1-Trichloroethane %RSE = 3.7




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 3510 | 2.5000 | 0.4553 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 16623 | 12.5000 | 0.4349 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 35547 | 25.0000 | 0.4492 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 67007 | 50.0000 | 0.4306 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 183324 | 125.0000 | 0.4576 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 174206 | 125.0000 | 0.4231 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 174206 | 125.0000 | 0.4231 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 386005 | 250.0000 | 0.4616 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 580748 | 375.0000 | 0.4599 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 778785 | 500.0000 | 0.4628 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:43 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

Dibromofluoromethane %RSE =

Dibromofluoromethane - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 2508 | 2.5000 | 0.3253 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 9074 | 12.5000 | 0.2374 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 19100 | 25.0000 | 0.2414 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 35309 | 50.0000 | 0.2269 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 89307 | 125.0000 | 0.2169 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 204707 | 250.0000 | 0.2555 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 204073 | 250.0000 | 0.2440 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 89307 | 250.0000 | 0.1084 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 305158 | 375.0000 | 0.2416 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 404568 | 500.0000 | 0.2404 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:43 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

Carbon tetrachloride %RSE = 3.9




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 4342 | 2.5000 | 0.5632 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 16466 | 12.5000 | 0.4308 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 34462 | 25.0000 | 0.4355 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 65313 | 50.0000 | 0.4197 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 181384 | 125.0000 | 0.4528 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 172928 | 125.0000 | 0.4200 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 172928 | 125.0000 | 0.4200 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 383485 | 250.0000 | 0.4586 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 572545 | 375.0000 | 0.4534 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 770907 | 500.0000 | 0.4581 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:44 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

1,1-Dichloropropene %RSE = 6.8




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 2830 | 2.5000 | 0.3671 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 13149 | 12.5000 | 0.3440 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 29241 | 25.0000 | 0.3695 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 56376 | 50.0000 | 0.3623 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 150930 | 125.0000 | 0.3768 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 149649 | 125.0000 | 0.3635 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 149649 | 125.0000 | 0.3635 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 335741 | 250.0000 | 0.4015 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 507157 | 375.0000 | 0.4016 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 693669 | 500.0000 | 0.4122 | |

Calibration Report

| | | | |
|---------------------|---|----------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:44 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

1,2-Dichloroethane-d4 %RSE =




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 923 | 2.5000 | 0.1198 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 3938 | 12.5000 | 0.1030 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 8284 | 25.0000 | 0.1047 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 15238 | 50.0000 | 0.0979 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 39086 | 125.0000 | 0.0949 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 91382 | 250.0000 | 0.1141 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 87876 | 250.0000 | 0.1051 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 39086 | 250.0000 | 0.0475 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 129608 | 375.0000 | 0.1026 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 174713 | 500.0000 | 0.1038 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:44 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

Benzene %RSE = 5.4

Benzene - 8 Levels, 8 Levels Used, 8 Points, 8 Points Used, 1 QCs




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|---------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | x | 8408 | 2.5000 | 1.0907 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 37071 | 12.5000 | 0.9699 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 74956 | 25.0000 | 0.9473 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 148727 | 50.0000 | 0.9557 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 418900 | 125.0000 | 1.0457 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 383469 | 125.0000 | 0.9313 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 383469 | 125.0000 | 0.9313 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 857534 | 250.0000 | 1.0254 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 1293370 | 375.0000 | 1.0242 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 1714050 | 500.0000 | 1.0186 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:44 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

1,2-Dichloroethane %RSE = 7.0




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | x | 2415 | 2.5000 | 0.3133 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 10202 | 12.5000 | 0.2669 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 19996 | 25.0000 | 0.2527 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 41058 | 50.0000 | 0.2638 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 104249 | 125.0000 | 0.2602 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 104855 | 125.0000 | 0.2547 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 104855 | 125.0000 | 0.2547 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 226964 | 250.0000 | 0.2714 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 332775 | 375.0000 | 0.2635 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 450739 | 500.0000 | 0.2679 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:44 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

Trichloroethene %RSE = 5.6




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 2372 | 2.5000 | 0.8011 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 10442 | 12.5000 | 0.7042 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 21946 | 25.0000 | 0.7283 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 42682 | 50.0000 | 0.7105 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 121734 | 125.0000 | 0.7908 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 114123 | 125.0000 | 0.7447 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 114123 | 125.0000 | 0.7447 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 250285 | 250.0000 | 0.7910 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 374370 | 375.0000 | 0.7932 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 505400 | 500.0000 | 0.8058 | |

Calibration Report

| | | | |
|---------------------|---|----------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:44 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

1,2-Dichloropropane %RSE = 3.7




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 2148 | 2.5000 | 0.7255 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 9488 | 12.5000 | 0.6399 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 20077 | 25.0000 | 0.6663 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 37870 | 50.0000 | 0.6304 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 102633 | 125.0000 | 0.6667 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 99187 | 125.0000 | 0.6472 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 99187 | 125.0000 | 0.6472 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 213800 | 250.0000 | 0.6757 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 324602 | 375.0000 | 0.6877 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 436057 | 500.0000 | 0.6953 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:44 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

Dibromomethane %RSE = 6.3

Dibromomethane - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 902 | 2.5000 | 0.3045 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 4675 | 12.5000 | 0.3153 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 8055 | 25.0000 | 0.2673 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 15989 | 50.0000 | 0.2662 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 43248 | 125.0000 | 0.2810 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 40628 | 125.0000 | 0.2651 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 40628 | 125.0000 | 0.2651 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 89483 | 250.0000 | 0.2828 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 134282 | 375.0000 | 0.2845 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 176038 | 500.0000 | 0.2807 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:44 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

Bromodichloromethane %RSE = 3.5

Bromodichloromethane - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 2536 | 2.5000 | 0.8565 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 11562 | 12.5000 | 0.7798 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 22743 | 25.0000 | 0.7547 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 43900 | 50.0000 | 0.7308 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 122757 | 125.0000 | 0.7975 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 115664 | 125.0000 | 0.7548 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 115664 | 125.0000 | 0.7548 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 251805 | 250.0000 | 0.7958 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 375983 | 375.0000 | 0.7966 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 502929 | 500.0000 | 0.8019 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:44 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

cis-1,3-Dichloropropene %RSE = 6.7

cis-1,3-Dichloropropene - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 2583 | 2.5000 | 0.8724 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 12525 | 12.5000 | 0.8447 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 24511 | 25.0000 | 0.8134 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 48886 | 50.0000 | 0.8138 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 130910 | 125.0000 | 0.8504 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 129419 | 125.0000 | 0.8445 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 129419 | 125.0000 | 0.8445 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 293617 | 250.0000 | 0.9280 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 441168 | 375.0000 | 0.9347 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 591147 | 500.0000 | 0.9426 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:44 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

Toluene-d8 %RSE =




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|---------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 7777 | 2.5000 | 2.6266 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 32318 | 12.5000 | 2.1796 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 67673 | 25.0000 | 2.2458 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 136453 | 50.0000 | 2.2715 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 358186 | 125.0000 | 2.3373 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 821531 | 250.0000 | 2.6685 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 823306 | 250.0000 | 2.6021 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 358186 | 250.0000 | 1.1687 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 1229775 | 375.0000 | 2.6054 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 1644540 | 500.0000 | 2.6222 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:44 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

Toluene %RSE = 6.5




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|---------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | x | 5039 | 2.5000 | 1.7019 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 21794 | 12.5000 | 1.4698 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 46355 | 25.0000 | 1.5383 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 91915 | 50.0000 | 1.5301 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 264584 | 125.0000 | 1.7188 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 244712 | 125.0000 | 1.5969 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 244712 | 125.0000 | 1.5969 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 541945 | 250.0000 | 1.7129 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 813204 | 375.0000 | 1.7229 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 1095161 | 500.0000 | 1.7462 | |

Calibration Report

| | | | |
|---------------------|---|----------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:44 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

trans-1,3-Dichloropropene %RSE = 6.2




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 1470 | 2.5000 | 0.4966 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 8683 | 12.5000 | 0.5856 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 17850 | 25.0000 | 0.5924 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 35179 | 50.0000 | 0.5856 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 98907 | 125.0000 | 0.6425 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 92719 | 125.0000 | 0.6050 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 92719 | 125.0000 | 0.6050 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 207833 | 250.0000 | 0.6569 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 315063 | 375.0000 | 0.6675 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 416771 | 500.0000 | 0.6645 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:44 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

1,1,2-Trichloroethane %RSE = 4.0




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 960 | 2.5000 | 0.3244 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 5090 | 12.5000 | 0.3433 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 10099 | 25.0000 | 0.3351 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 18884 | 50.0000 | 0.3144 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 49128 | 125.0000 | 0.3191 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 46673 | 125.0000 | 0.3046 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 46673 | 125.0000 | 0.3046 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 101888 | 250.0000 | 0.3220 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 152331 | 375.0000 | 0.3227 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 205463 | 500.0000 | 0.3276 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:44 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

Tetrachloroethene %RSE = 5.2




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | x | 2105 | 2.5000 | 0.7110 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 9238 | 12.5000 | 0.6230 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 20322 | 25.0000 | 0.6744 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 36925 | 50.0000 | 0.6147 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 103027 | 125.0000 | 0.6693 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 97590 | 125.0000 | 0.6368 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 97590 | 125.0000 | 0.6368 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 218245 | 250.0000 | 0.6898 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 319950 | 375.0000 | 0.6779 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 428812 | 500.0000 | 0.6837 | |

Calibration Report

| | | | |
|---------------------|---|----------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:44 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

1,3-Dichloropropane %RSE = 3.9




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 2257 | 2.5000 | 0.7623 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 8967 | 12.5000 | 0.6047 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 18745 | 25.0000 | 0.6221 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 37457 | 50.0000 | 0.6235 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 95697 | 125.0000 | 0.6217 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 96183 | 125.0000 | 0.6276 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 96183 | 125.0000 | 0.6276 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 212669 | 250.0000 | 0.6722 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 312547 | 375.0000 | 0.6622 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 408993 | 500.0000 | 0.6521 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:44 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

Chlorodibromomethane %RSE = 4.5

Chlorodibromomethane - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 1468 | 2.5000 | 0.4958 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 7718 | 12.5000 | 0.5205 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 14873 | 25.0000 | 0.4936 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 28153 | 50.0000 | 0.4687 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 78076 | 125.0000 | 0.5072 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 75015 | 125.0000 | 0.4895 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 75015 | 125.0000 | 0.4895 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 165695 | 250.0000 | 0.5237 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 247279 | 375.0000 | 0.5239 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 330813 | 500.0000 | 0.5275 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:44 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

1,2-Dibromoethane %RSE = 2.9




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 1299 | 2.5000 | 0.4388 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 5410 | 12.5000 | 0.3649 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 10410 | 25.0000 | 0.3455 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 21037 | 50.0000 | 0.3502 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 54259 | 125.0000 | 0.3525 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 51827 | 125.0000 | 0.3382 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 51827 | 125.0000 | 0.3382 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 115714 | 250.0000 | 0.3657 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 168577 | 375.0000 | 0.3572 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 225877 | 500.0000 | 0.3602 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:44 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

Chlorobenzene %RSE = 3.5

Chlorobenzene - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|---------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 5771 | 2.5000 | 1.9491 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 26461 | 12.5000 | 1.7846 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 53047 | 25.0000 | 1.7604 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 101452 | 50.0000 | 1.6889 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 288815 | 125.0000 | 1.8762 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 263617 | 125.0000 | 1.7202 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 263617 | 125.0000 | 1.7202 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 582326 | 250.0000 | 1.8405 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 867732 | 375.0000 | 1.8384 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 1153147 | 500.0000 | 1.8387 | |

Calibration Report

| | | | |
|---------------------|---|----------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:44 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

1,1,1,2-Tetrachloroethane %RSE = 4.2




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 1893 | 2.5000 | 0.6392 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 9473 | 12.5000 | 0.6389 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 18130 | 25.0000 | 0.6016 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 35544 | 50.0000 | 0.5917 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 97148 | 125.0000 | 0.6311 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 90898 | 125.0000 | 0.5932 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 90898 | 125.0000 | 0.5932 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 200859 | 250.0000 | 0.6348 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 307436 | 375.0000 | 0.6513 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 406450 | 500.0000 | 0.6481 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:45 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

Ethylbenzene %RSE = 7.5

Ethylbenzene - 8 Levels, 8 Levels Used, 8 Points, 8 Points Used, 1 QCs




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|---------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | x | 9283 | 2.5000 | 3.1353 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 40470 | 12.5000 | 2.7294 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 88428 | 25.0000 | 2.9345 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 173769 | 50.0000 | 2.8927 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 501953 | 125.0000 | 3.2608 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 464148 | 125.0000 | 3.0288 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 464148 | 125.0000 | 3.0288 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 1043443 | 250.0000 | 3.2979 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 1574219 | 375.0000 | 3.3352 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 2111152 | 500.0000 | 3.3662 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:45 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

m+p-Xylenes %RSE = 8.3




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|---------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | x | 7212 | 5.0000 | 1.2179 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 31538 | 25.0000 | 1.0635 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 66267 | 50.0000 | 1.0995 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 133498 | 100.0000 | 1.1112 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 388558 | 250.0000 | 1.2621 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 368418 | 250.0000 | 1.2021 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 368418 | 250.0000 | 1.2021 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 825866 | 500.0000 | 1.3051 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 1228570 | 750.0000 | 1.3014 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 1637879 | 1000.0000 | 1.3058 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:45 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

o-Xylene %RSE = 9.2

o-Xylene - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 3330 | 2.5000 | 1.1247 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 13519 | 12.5000 | 0.9117 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 30463 | 25.0000 | 1.0109 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 61016 | 50.0000 | 1.0157 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 174061 | 125.0000 | 1.1308 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 161509 | 125.0000 | 1.0539 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 161509 | 125.0000 | 1.0539 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 365914 | 250.0000 | 1.1565 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 549244 | 375.0000 | 1.1636 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 734101 | 500.0000 | 1.1705 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:45 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

Styrene %RSE = 9.9

Styrene - 8 Levels, 8 Levels Used, 8 Points, 8 Points Used, 1 QCs




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|---------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | x | 4408 | 2.5000 | 1.4888 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 23472 | 12.5000 | 1.5830 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 48569 | 25.0000 | 1.6118 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 96576 | 50.0000 | 1.6077 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 291425 | 125.0000 | 1.8932 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 268375 | 125.0000 | 1.7513 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 268375 | 125.0000 | 1.7513 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 605646 | 250.0000 | 1.9142 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 896331 | 375.0000 | 1.8990 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 1199879 | 500.0000 | 1.9132 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:45 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

Bromoform %RSE = 4.7

Bromoform - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 708 | 2.5000 | 0.3108 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 3652 | 12.5000 | 0.3016 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 7972 | 25.0000 | 0.3317 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 16073 | 50.0000 | 0.3232 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 42560 | 125.0000 | 0.3326 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 39165 | 125.0000 | 0.2962 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 39165 | 125.0000 | 0.2962 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 87836 | 250.0000 | 0.3295 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 129038 | 375.0000 | 0.3227 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 175918 | 500.0000 | 0.3345 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:45 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

p-Bromofluorobenzene %RSE =




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 2719 | 2.5000 | 1.1932 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 10059 | 12.5000 | 0.8308 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 22267 | 25.0000 | 0.9265 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 42506 | 50.0000 | 0.8548 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 114269 | 125.0000 | 0.8641 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 253034 | 250.0000 | 0.9888 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 261042 | 250.0000 | 0.9793 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 114269 | 250.0000 | 0.4321 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 385474 | 375.0000 | 0.9639 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 521580 | 500.0000 | 0.9917 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:45 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

Bromobenzene %RSE = 3.9




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 2024 | 2.5000 | 0.8880 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 9663 | 12.5000 | 0.7981 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 19259 | 25.0000 | 0.8013 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 38282 | 50.0000 | 0.7698 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 109054 | 125.0000 | 0.8523 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 102265 | 125.0000 | 0.7733 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 102265 | 125.0000 | 0.7733 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 227127 | 250.0000 | 0.8521 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 333431 | 375.0000 | 0.8338 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 439147 | 500.0000 | 0.8350 | |

Calibration Report

| | | | |
|---------------------|---|----------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:45 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

1,1,2,2-Tetrachloroethane %RSE = 5.8




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 1142 | 2.5000 | 0.5014 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 5793 | 12.5000 | 0.4785 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 12440 | 25.0000 | 0.5176 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 22514 | 50.0000 | 0.4528 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 60763 | 125.0000 | 0.4749 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 56958 | 125.0000 | 0.4307 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 56958 | 125.0000 | 0.4307 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 124205 | 250.0000 | 0.4660 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 182470 | 375.0000 | 0.4563 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 240837 | 500.0000 | 0.4579 | |

Calibration Report

| | | | |
|---------------------|---|----------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:45 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

1,2,3-Trichloropropane %RSE = 6.5




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|-------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 1654 | 12.5000 | 0.1366 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 3200 | 25.0000 | 0.1331 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 6096 | 50.0000 | 0.1226 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 15682 | 125.0000 | 0.1226 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 14846 | 125.0000 | 0.1123 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 14846 | 125.0000 | 0.1123 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 33115 | 250.0000 | 0.1242 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 48325 | 375.0000 | 0.1208 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 64422 | 500.0000 | 0.1225 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:45 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

2-Chlorotoluene %RSE = 6.8

2-Chlorotoluene - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 1844 | 2.5000 | 0.8090 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 8731 | 12.5000 | 0.7211 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 19390 | 25.0000 | 0.8068 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 37987 | 50.0000 | 0.7639 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 108192 | 125.0000 | 0.8456 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 102424 | 125.0000 | 0.7745 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 102424 | 125.0000 | 0.7745 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 229396 | 250.0000 | 0.8606 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 336386 | 375.0000 | 0.8411 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 455991 | 500.0000 | 0.8670 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:45 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

4-Chlorotoluene %RSE = 6.5




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|---------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | | 5419 | 2.5000 | 2.3780 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 28532 | 12.5000 | 2.3566 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 61551 | 25.0000 | 2.5611 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 126308 | 50.0000 | 2.5400 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 368295 | 125.0000 | 2.8784 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 336146 | 125.0000 | 2.5420 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 336146 | 125.0000 | 2.5420 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 748435 | 250.0000 | 2.8078 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 1109221 | 375.0000 | 2.7736 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 1468376 | 500.0000 | 2.7919 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:45 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

1,3-Dichlorobenzene %RSE = 4.6




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | x | 3541 | 2.5000 | 1.5539 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 16932 | 12.5000 | 1.3985 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 36559 | 25.0000 | 1.5212 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 69539 | 50.0000 | 1.3984 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 204088 | 125.0000 | 1.5950 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 183404 | 125.0000 | 1.3869 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 183404 | 125.0000 | 1.3869 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 406895 | 250.0000 | 1.5265 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 603674 | 375.0000 | 1.5095 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 793993 | 500.0000 | 1.5097 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:45 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |

1,4-Dichlorobenzene %RSE = 5.0




| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | x | 3787 | 2.5000 | 1.6618 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 17438 | 12.5000 | 1.4403 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 36635 | 25.0000 | 1.5243 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 71841 | 50.0000 | 1.4447 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 200032 | 125.0000 | 1.5633 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 189045 | 125.0000 | 1.4296 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 189045 | 125.0000 | 1.4296 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 408934 | 250.0000 | 1.5342 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 595919 | 375.0000 | 1.4901 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 794954 | 500.0000 | 1.5115 | |

Calibration Report

| | | | |
|----------------------------|---|-----------------------------|----------------|
| Batch Path | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name | BL2000\mchavez |
| Analysis Time | 2/28/2022 1:57 PM | Reporter Name | BL2000\mchavez |
| Report Time | 2/28/2022 2:00:45 PM | Batch State | Processed |
| Last Calib Update | 1/9/2022 8:59 PM | Quant Report Version | 10.0 |
| Quant Batch Version | 10.0 | | |


1,2-Dichlorobenzene %RSE = 4.9



| Calibration STD Path | Cal Type | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|---|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D | Calibration | 1 | x | 3104 | 2.5000 | 1.3621 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D | Calibration | 2 | x | 14666 | 12.5000 | 1.2114 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D | Calibration | 3 | x | 29899 | 25.0000 | 1.2441 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D | Calibration | 4 | x | 60213 | 50.0000 | 1.2109 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D | QC | QC | x | 164299 | 125.0000 | 1.2841 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D | Calibration | 5 | x | 152284 | 125.0000 | 1.1516 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC | CC | x | 152284 | 125.0000 | 1.1516 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D | Calibration | 6 | x | 342576 | 250.0000 | 1.2852 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D | Calibration | 7 | x | 499147 | 375.0000 | 1.2481 | |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D | Calibration | 8 | x | 664247 | 500.0000 | 1.2630 | |

Quantitation Results Report (QT Reviewed)

| | | | |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File | 04JAN09.D | Operator | MSC |
| Acq. Method | 5975CACQF.M | Acq. Date-Time | 1/4/2022 3:05:37 PM |
| Sample Name | MBLK010422_ | Instrument | VOA5975C |
| Vial | 9 | Multiplier | 1.00 |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m | Comment | |
| Tune File | BFB_Atune3.u | Tune Date | 10/11/2021 4:02:00 PM |
| Batch Name | VG010422_8260B.batch.bin | Last Calib Update | 1/9/2022 8:59:52 PM |
| Ref Library | \\MASSHUNTER\Org\Library\NIST129K.I | | |











| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|--------------------|-------|----------|
| Internal Standards | | | | | | |
| M Fluorobenzene | 6.620 | 96.0 | 775552 | 250.0000 | ng | -0.003 |
| M Chlorobenzene-d5 | 9.774 | 82.0 | 301196 | 250.0000 | ng | 0.003 |
| M 1,4-Dichlorobenzene-d4 | 12.100 | 152.0 | 231562 | 250.0000 | ng | 0.000 |
| System Monitoring Compounds | | | | | | |
| S Dibromofluoromethane | 5.848 | 113.0 | 203459 | 278.4635 | ng | 0.003 |
| Spiked Amount: 250.000 | Range: 80.0 - 119.0% | | | Recovery = 111.39% | | |
| S 1,2-Dichloroethane-d4 | 6.233 | 67.0 | 88174 | 279.3964 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 81.0 - 118.0% | | | Recovery = 111.76% | | |
| S Toluene-d8 | 8.319 | 98.0 | 770154 | 265.3436 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 89.0 - 112.0% | | | Recovery = 106.14% | | |
| S p-Bromofluorobenzene | 10.951 | 95.0 | 226743 | 267.2815 | ng | -0.003 |
| Spiked Amount: 250.000 | Range: 85.0 - 114.0% | | | Recovery = 106.91% | | |
| Target Compounds | | | | | | |
| T Dichlorodifluoromethane | 0.000 | | 0 | N.D. | | |
| T Chloromethane | 1.333 | 50.0 | 0 | | ng | md 1 |
| T Vinyl chloride | 1.489 | 62.0 | 0 | | ng | md 1 |
| T Bromomethane | 0.000 | | 0 | N.D. | | |
| T Chloroethane | 0.000 | | 0 | N.D. | | |
| T Trichlorofluoromethane | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methylene chloride | 3.335 | 49.0 | 1661 | 1.4424 | ng | m 97 |
| T trans-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methyl tert-butyl ether (MTBE) | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloroethane | 0.000 | | 0 | N.D. | | |
| T 2,2-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T cis-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methyl ethyl ketone | 0.000 | | 0 | N.D. | | |
| T Bromochloromethane | 0.000 | | 0 | N.D. | | |
| T Chloroform | 0.000 | | 0 | N.D. | | |

Quantitation Results Report (QT Reviewed)




| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|-----------------------------|-------|------|-------|--------|-----------|----------|
| T 1,1,1-Trichloroethane | 0.000 | | 0 | N.D. | | |
| T Carbon tetrachloride | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloropropene | 0.000 | | 0 | N.D. | | |
| T Benzene | 6.266 | 78.0 | 381 | 0.1233 | ng m | 98 |
| T 1,2-Dichloroethane | 0.000 | | 0 | N.D. | | |
| T Trichloroethene | 0.000 | | 0 | N.D. | | |
| T 1,2-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T Dibromomethane | 0.000 | | 0 | N.D. | | |
| T Bromodichloromethane | 0.000 | | 0 | N.D. | | |
| T cis-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | |
| T Toluene | 0.000 | | 0 | N.D. | | |
| T trans-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | |
| T 1,1,2-Trichloroethane | 0.000 | | 0 | N.D. | | |
| T Tetrachloroethene | 0.000 | | 0 | N.D. | | |
| T 1,3-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T Chlorodibromomethane | 0.000 | | 0 | N.D. | | |
| T 1,2-Dibromoethane | 0.000 | | 0 | N.D. | | |
| T Chlorobenzene | 0.000 | | 0 | N.D. | | |
| T 1,1,1,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | |
| T Ethylbenzene | 0.000 | | 0 | N.D. | | |
| T m+p-Xylenes | 0.000 | | 0 | N.D. | | |
| T o-Xylene | 0.000 | | 0 | N.D. | | |
| T Styrene | 0.000 | | 0 | N.D. | | |
| T Bromoform | 0.000 | | 0 | N.D. | | |
| T Bromobenzene | 0.000 | | 0 | N.D. | | |
| T 1,1,2,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | |
| T 1,2,3-Trichloropropane | 0.000 | | 0 | N.D. | | |
| T 2-Chlorotoluene | 0.000 | | 0 | N.D. | | |
| T 4-Chlorotoluene | 0.000 | | 0 | N.D. | | |
| T 1,3-Dichlorobenzene | 0.000 | | 0 | N.D. | | |
| T 1,4-Dichlorobenzene | 0.000 | | 0 | N.D. | | |
| T 1,2-Dichlorobenzene | 0.000 | | 0 | N.D. | | |

(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak


Quantitation Results Report (QT Reviewed)
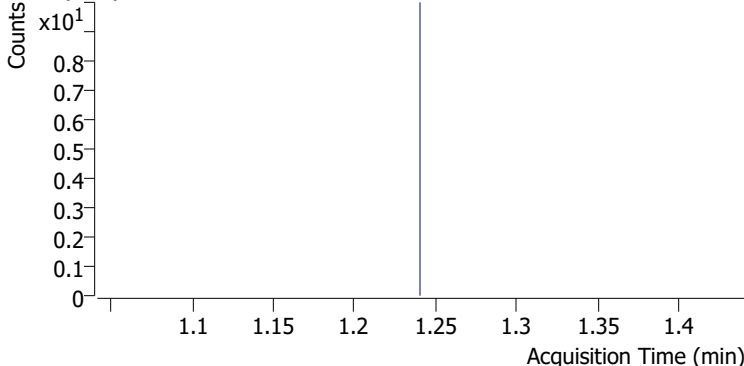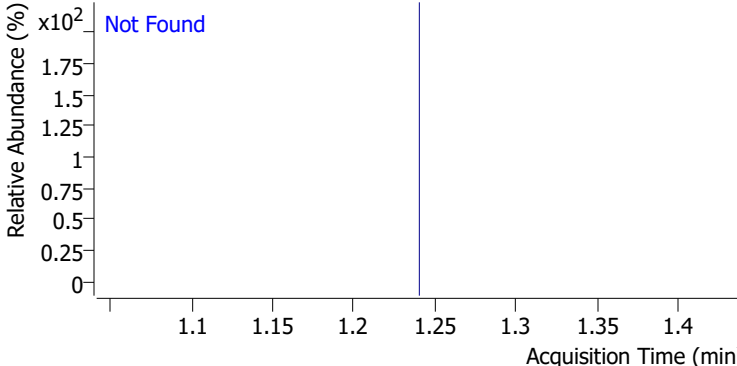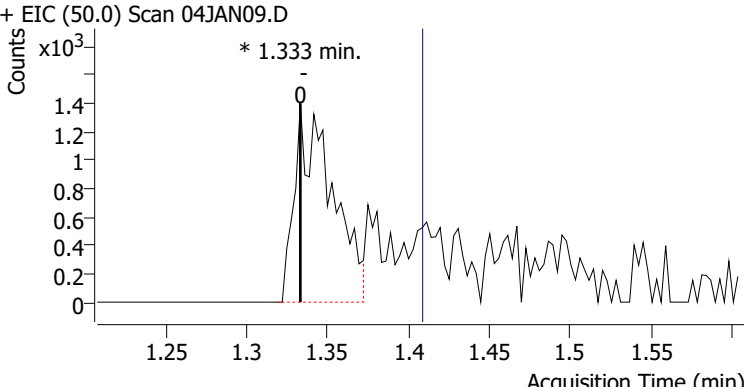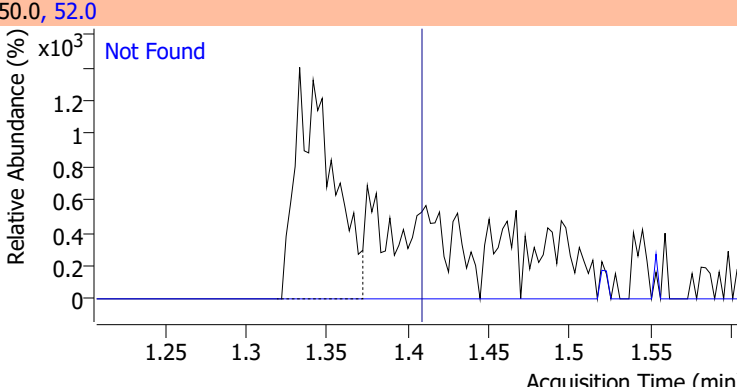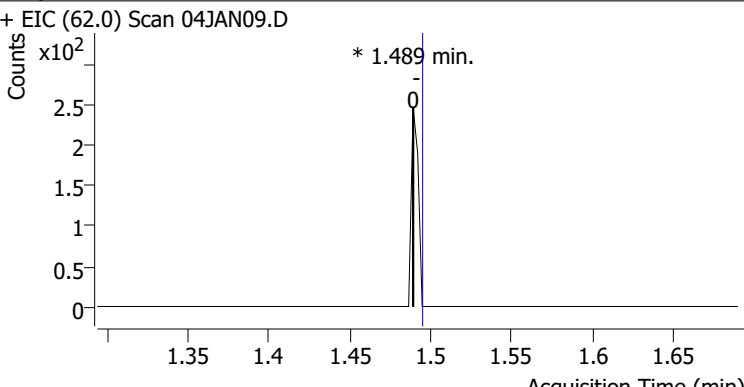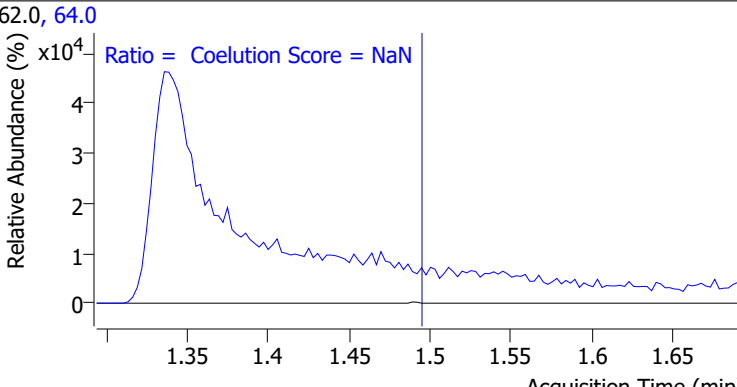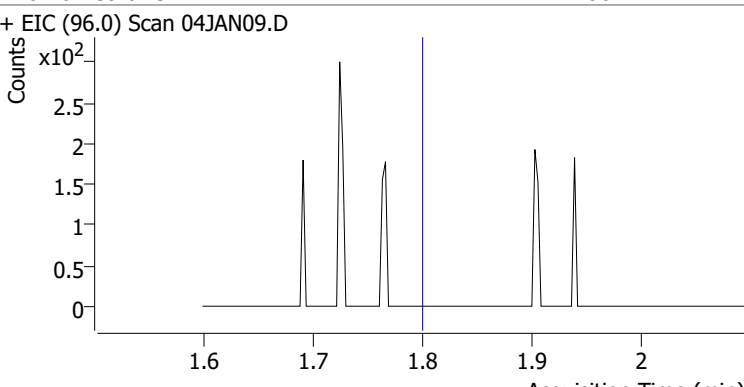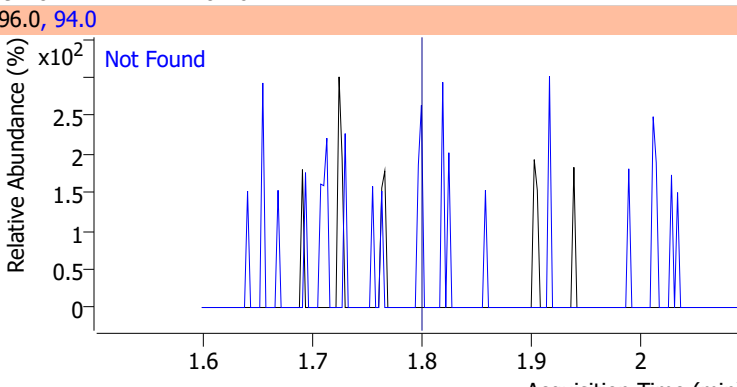
| Compound | Conc. | Exp RT | QIon | Exp Ratio | | | | |
|--|-------|--------|----------|-----------|------|--------|-------|-------|
| Dichlorodifluoromethane | N.D. | 1.24 | 87.0 | 32.3 | | | | |
| <div style="display: flex; justify-content: space-between;"> <div style="width: 48%;"> <p>+ EIC (85.0) Scan 04JAN09.D ***NO DATA POINTS***</p>  </div> <div style="width: 48%;"> <p>85.0, 87.0</p>  <p style="color: blue;">Not Found</p> </div> </div> | | | | | | | | |
| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
| Chloromethane | 0 | 1.333 | 0 | 0 | 52.0 | - | 2.1 | 62.1 |
| <div style="display: flex; justify-content: space-between;"> <div style="width: 48%;"> <p>+ EIC (50.0) Scan 04JAN09.D</p> <p>* 1.333 min.</p>  </div> <div style="width: 48%;"> <p>50.0, 52.0</p>  <p style="color: blue;">Not Found</p> </div> </div> | | | | | | | | |
| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
| Vinyl chloride | 0 | 1.489 | 0 | 0 | 64.0 | - | 0.0 | 59.9 |
| <div style="display: flex; justify-content: space-between;"> <div style="width: 48%;"> <p>+ EIC (62.0) Scan 04JAN09.D</p> <p>* 1.489 min.</p>  </div> <div style="width: 48%;"> <p>62.0, 64.0</p> <p style="color: blue;">Ratio = Coelution Score = NaN</p>  </div> </div> | | | | | | | | |
| Compound | Conc. | Exp RT | QIon | Exp Ratio | | | | |
| Bromomethane | N.D. | 1.80 | 94.0 | 104.6 | | | | |
| <div style="display: flex; justify-content: space-between;"> <div style="width: 48%;"> <p>+ EIC (96.0) Scan 04JAN09.D</p>  </div> <div style="width: 48%;"> <p>96.0, 94.0</p>  <p style="color: blue;">Not Found</p> </div> </div> | | | | | | | | |

Quantitation Results Report (QT Reviewed)

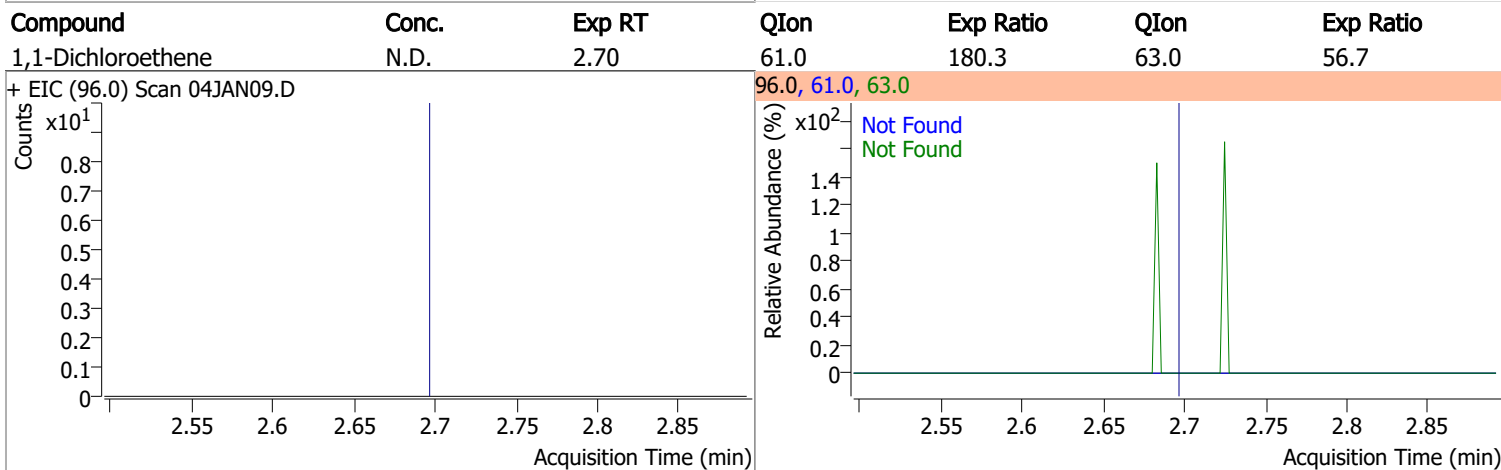


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|--------|------|----------|----------|------|--------|-------|-------|
| Methylene chloride | 1.4424 | 3.34 | 0.00 | 1661 (m) | 84.0 | 64.7 | 36.9 | 96.9 |
| | | | | | 86.0 | 41.8 | 14.3 | 74.3 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,2-Dichloroethene | N.D. | 3.72 | 61.0 | 153.9 | 98.0 | 65.7 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------------------|-------|--------|------|-----------|
| Methyl tert-butyl ether (MTBE) | N.D. | 3.75 | 57.0 | 24.6 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethane | N.D. | 4.38 | 65.0 | 32.1 | 83.0 | 13.7 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|------|-----------|
| 2,2-Dichloropropane | N.D. | 5.20 | 41.0 | 66.5 | 97.0 | 23.2 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|------------------------|-------|--------|------|-----------|------|-----------|
| cis-1,2-Dichloroethene | N.D. | 5.22 | 61.0 | 167.2 | 98.0 | 67.3 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| Methyl ethyl ketone | N.D. | 5.28 | 72.0 | 21.3 |







| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|
| Bromochloromethane | N.D. | 5.52 | 49.0 | 182.9 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|------------|-------|--------|------|-----------|
| Chloroform | N.D. | 5.65 | 85.0 | 66.0 |




Quantitation Results Report (QT Reviewed)

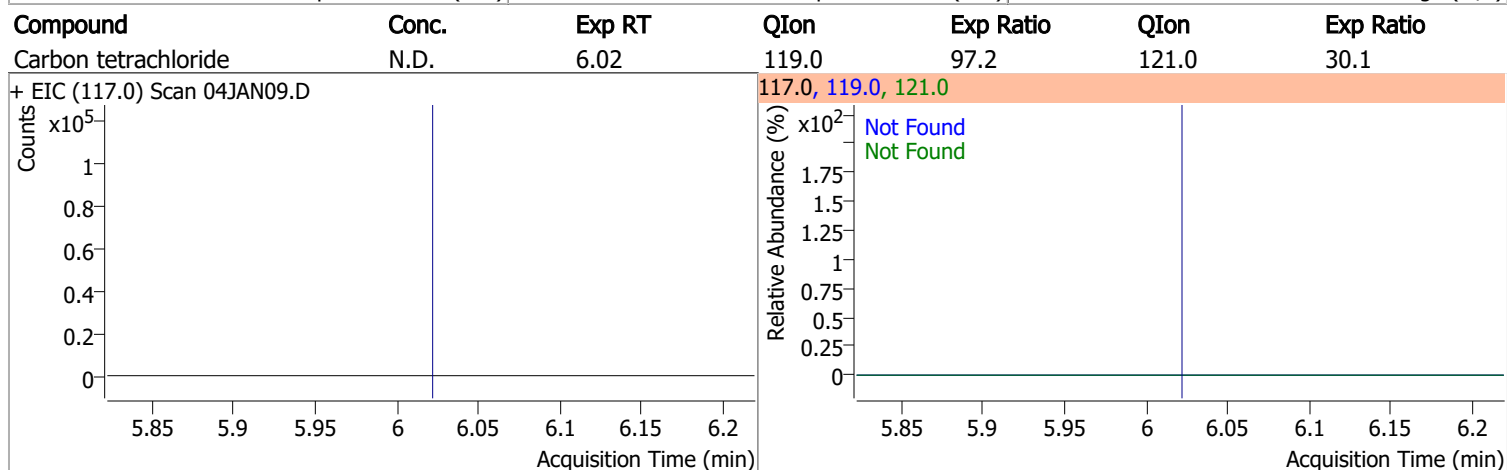


Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 279.3964 | 6.23 | 0.00 | 88174 | 65.0 | 198.1 | 166.5 | 226.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|--------|------|----------|---------|------|--------|-------|-------|
| Benzene | 0.1233 | 6.27 | -0.01 | 381 (m) | 77.0 | 22.7 | 0.0 | 53.5 |







| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,2-Dichloroethane | N.D. | 6.32 | 64.0 | 29.9 | 98.0 | 7.6 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------|-------|--------|-------|-----------|------|-----------|
| Trichloroethene | N.D. | 7.03 | 130.0 | 101.5 | 97.0 | 64.1 |




Quantitation Results Report (QT Reviewed)

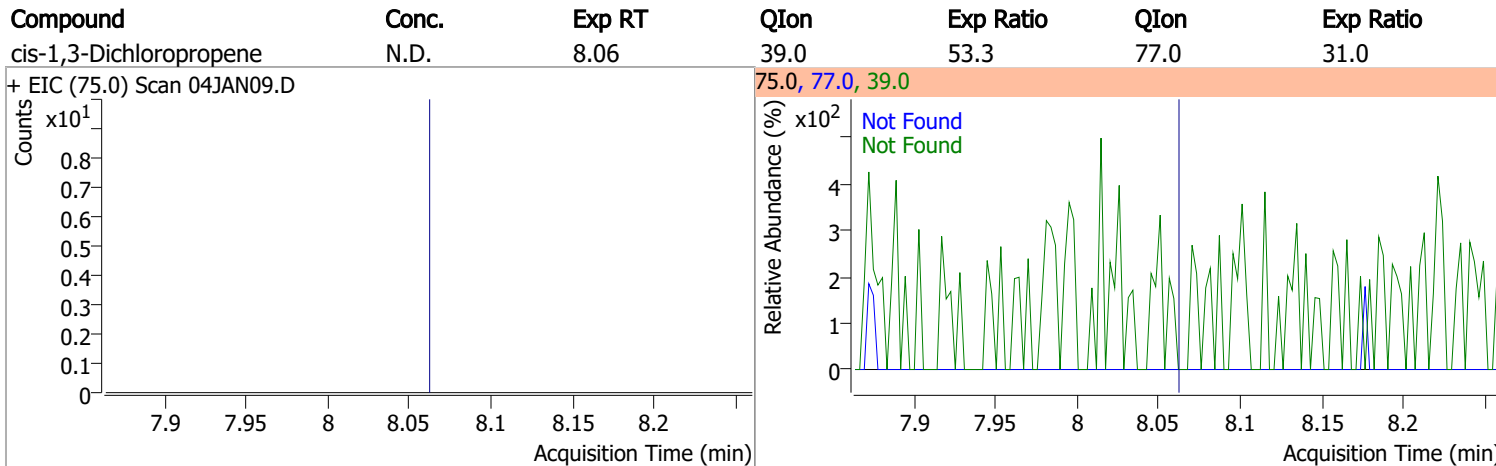


Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 265.3436 | 8.32 | 0.00 | 770154 | 100.0 | 64.0 | 34.4 | 94.4 |
| | | | | | 99.0 | 9.8 | 0.0 | 39.6 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------|-------|--------|------|-----------|
| Toluene | N.D. | 8.39 | 91.0 | 175.8 |











| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,3-Dichloropropene | N.D. | 8.64 | 39.0 | 53.4 | 77.0 | 32.4 |











| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------------|-------|--------|------|-----------|------|-----------|
| 1,1,2-Trichloroethane | N.D. | 8.82 | 97.0 | 114.6 | 85.0 | 67.6 |






Quantitation Results Report (QT Reviewed)
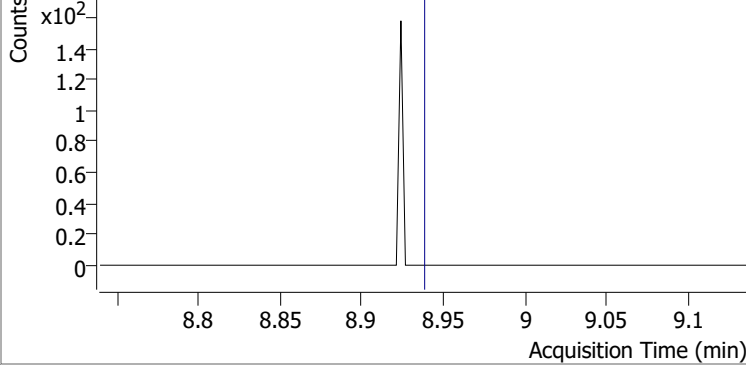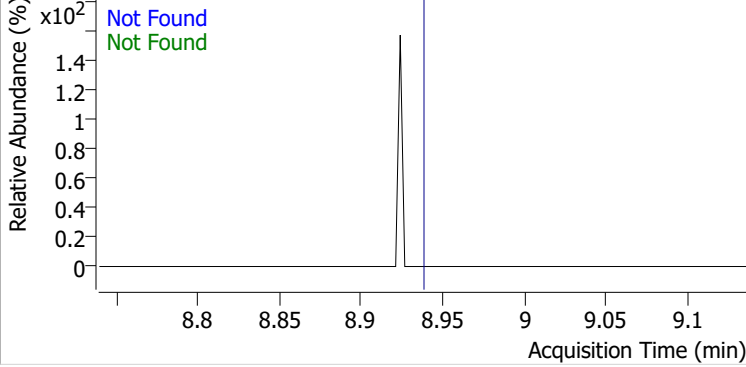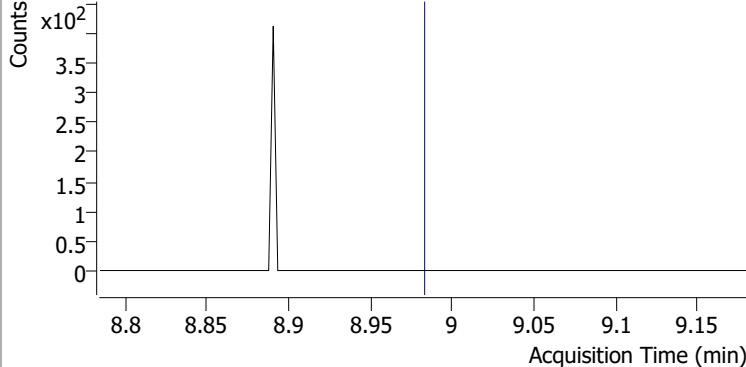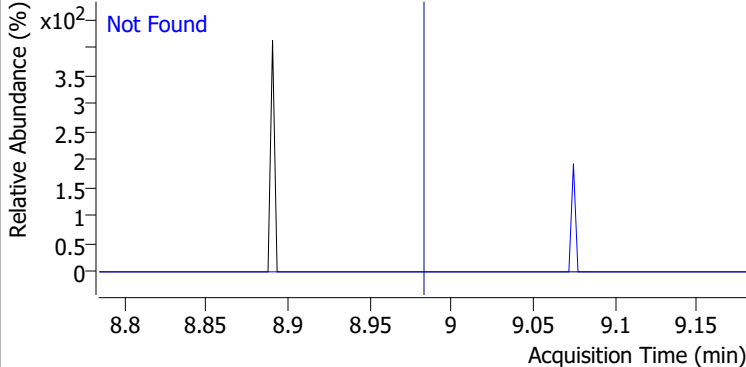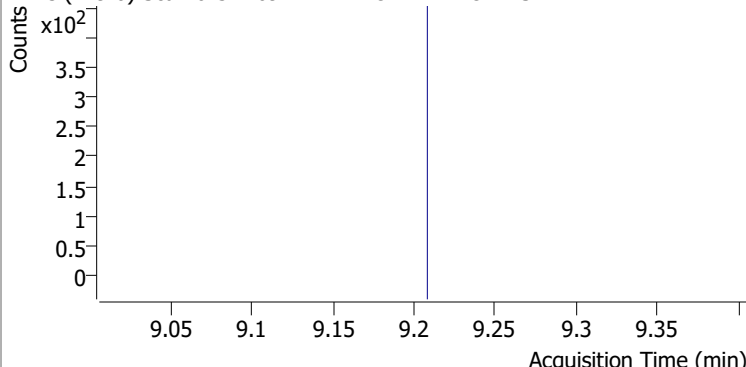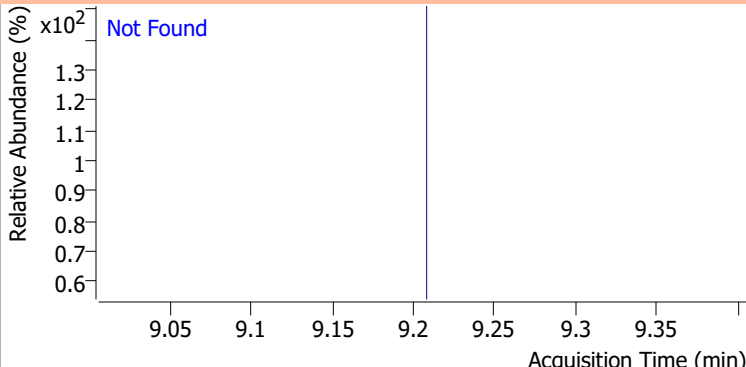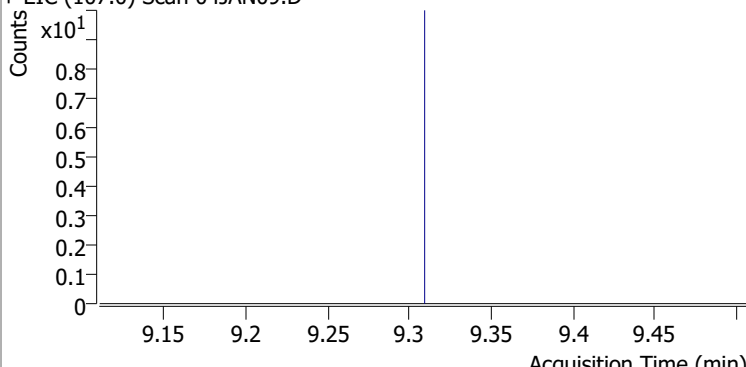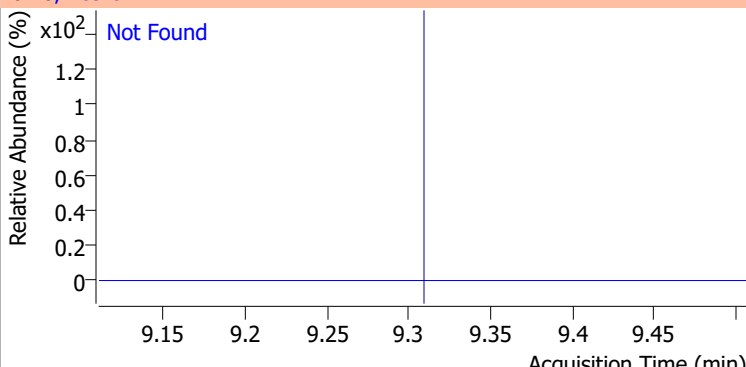
| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--|-------|--------|--|-----------|-------|-----------|
| Tetrachloroethene | N.D. | 8.94 | 165.8 | 128.6 | 129.0 | 91.5 |
| + EIC (163.8) Scan 04JAN09.D | | | 163.8, 129.0, 165.8 | | | |
|  | | |  | | | |
| 1,3-Dichloropropane | N.D. | 8.98 | 78.0 | 32.9 | | |
| + EIC (76.0) Scan 04JAN09.D | | | 76.0, 78.0 | | | |
|  | | |  | | | |
| Chlorodibromomethane | N.D. | 9.21 | 127.0 | 78.0 | | |
| + EIC (129.0) Scan 04JAN09.D ***NO DATA POINTS*** | | | 129.0, 127.0 | | | |
|  | | |  | | | |
| 1,2-Dibromoethane | N.D. | 9.31 | 109.0 | 94.5 | | |
| + EIC (107.0) Scan 04JAN09.D | | | 107.0, 109.0 | | | |
|  | | |  | | | |


Quantitation Results Report (QT Reviewed)
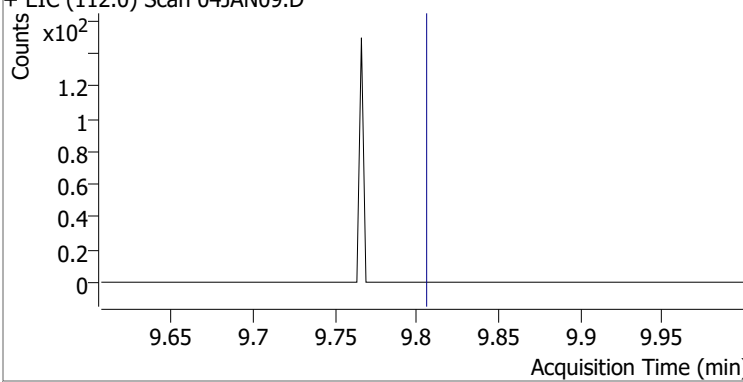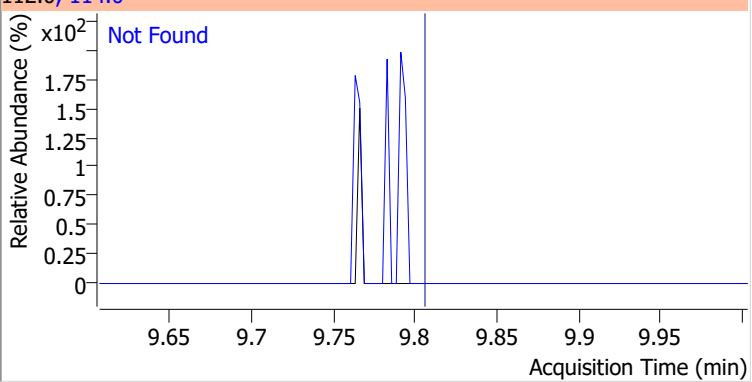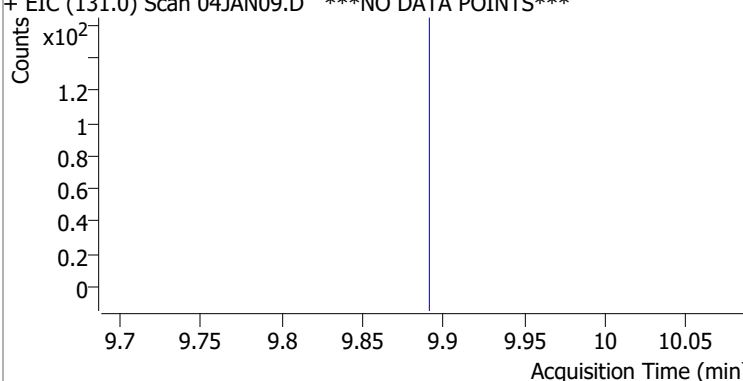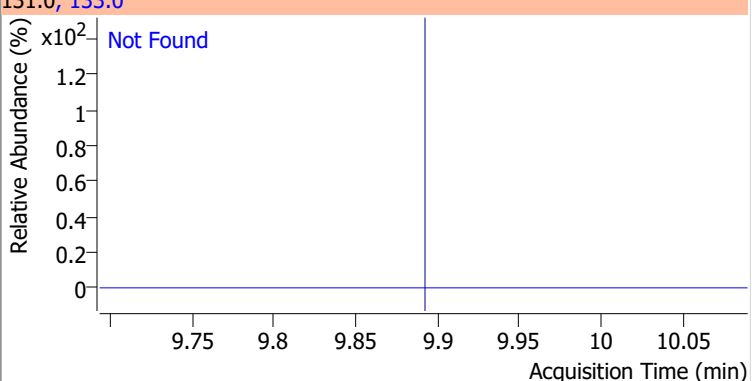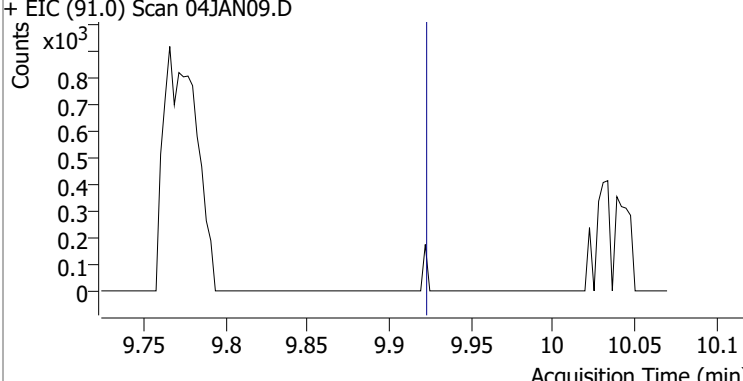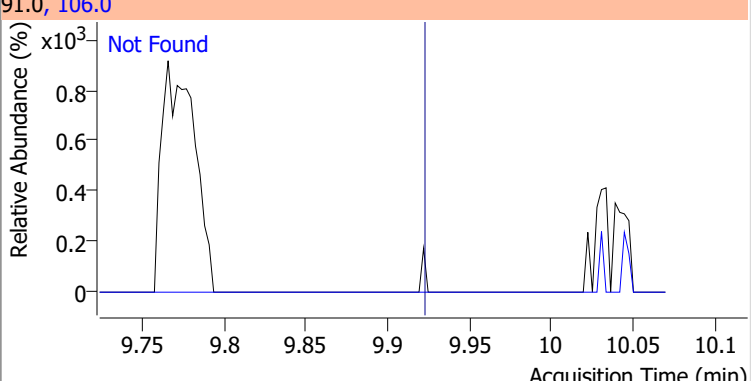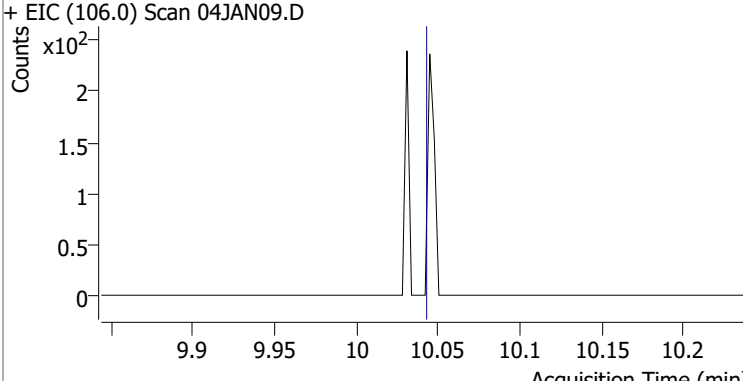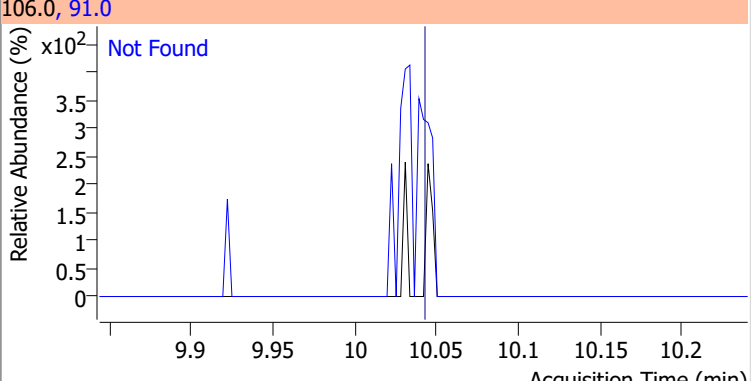
| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--|-------|--------|---|-----------|
| Chlorobenzene | N.D. | 9.80 | 114.0 | 32.1 |
| + EIC (112.0) Scan 04JAN09.D  | | | 112.0, 114.0  | |
| 1,1,1,2-Tetrachloroethane | N.D. | 9.89 | 133.0 | 98.6 |
| + EIC (131.0) Scan 04JAN09.D ***NO DATA POINTS***  | | | 131.0, 133.0  | |
| Ethylbenzene | N.D. | 9.92 | 106.0 | 31.1 |
| + EIC (91.0) Scan 04JAN09.D  | | | 91.0, 106.0  | |
| m+p-Xylenes | N.D. | 10.04 | 91.0 | 201.4 |
| + EIC (106.0) Scan 04JAN09.D  | | | 106.0, 91.0  | |









Quantitation Results Report (QT Reviewed)

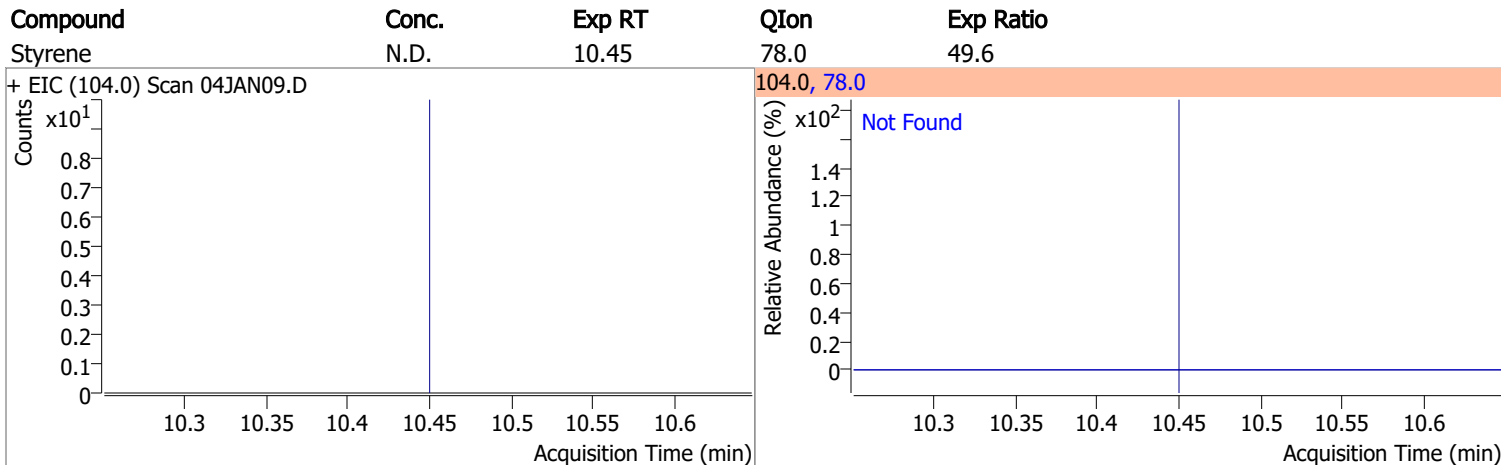









| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 267.2815 | 10.95 | 0.00 | 226743 | 174.0 | 95.5 | 61.7 | 121.7 |
| | | | | | 176.0 | 91.1 | 60.6 | 120.6 |



Quantitation Results Report (QT Reviewed)

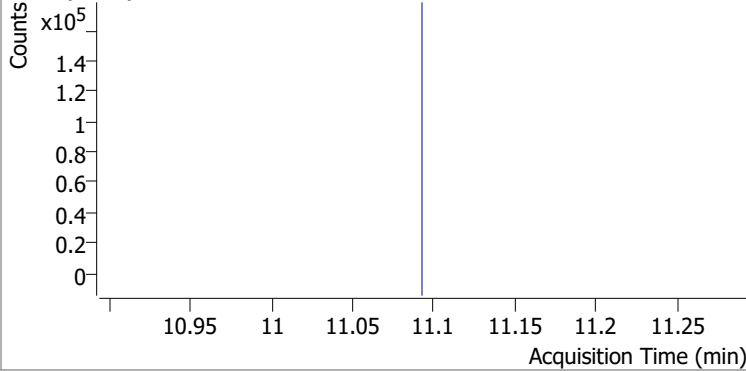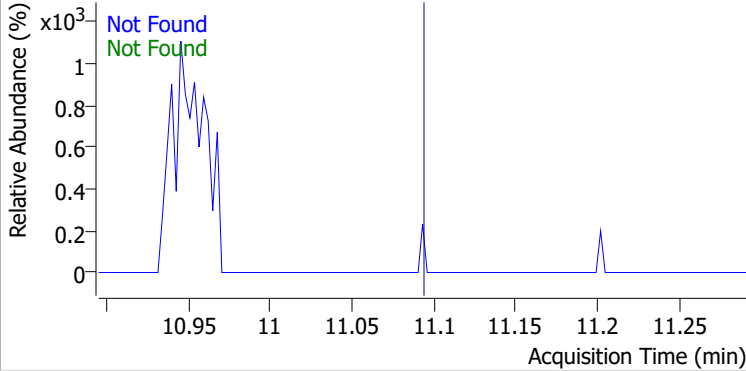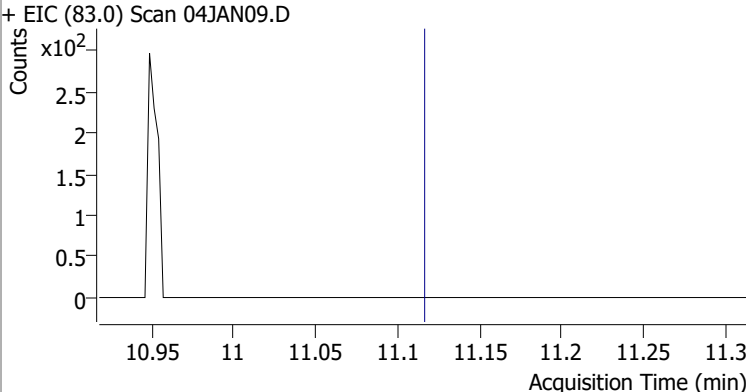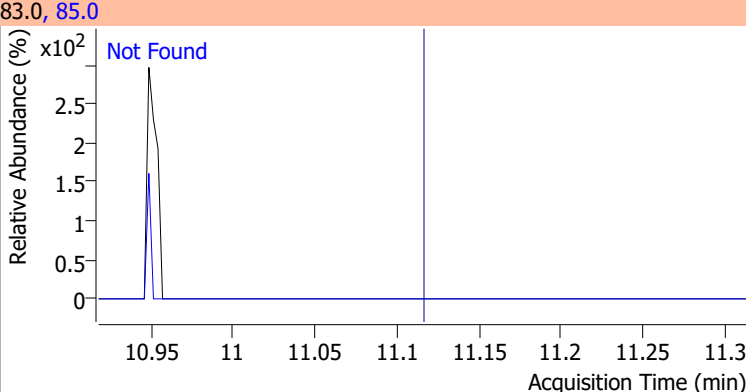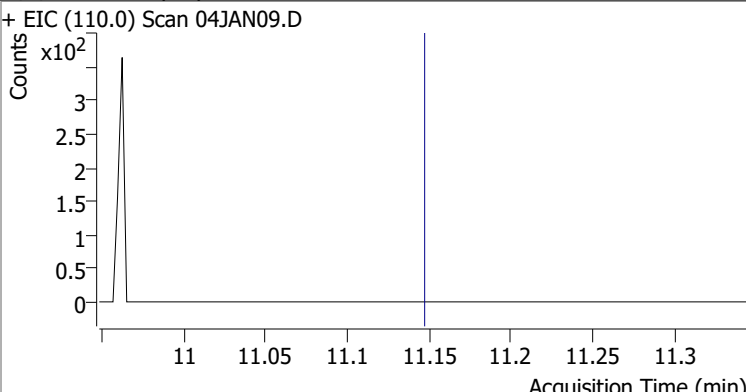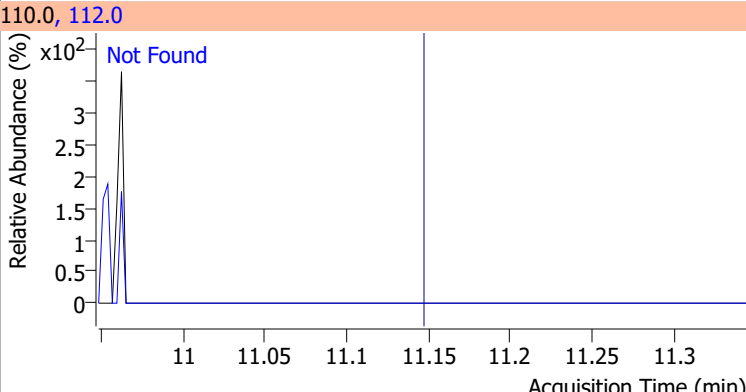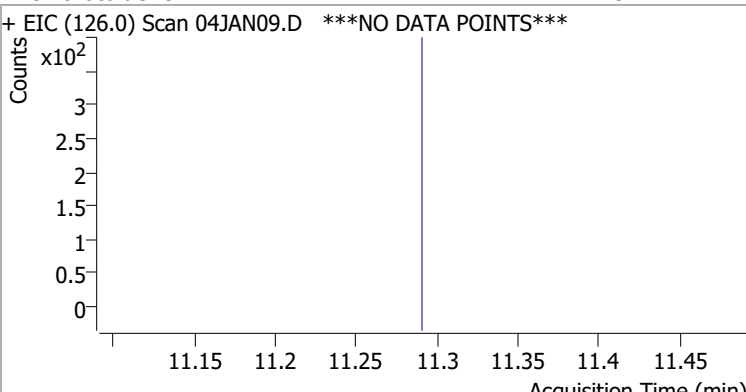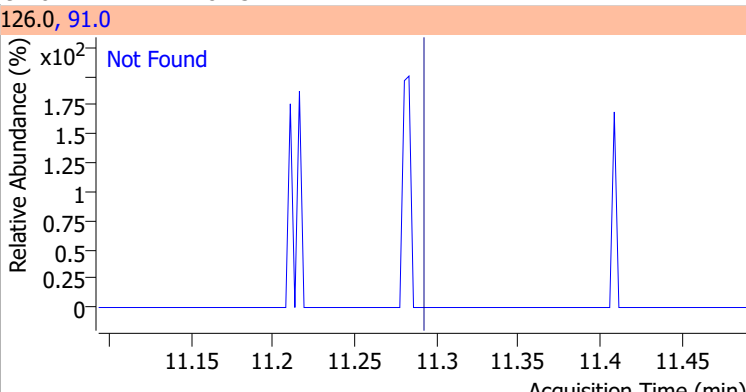
| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--|-------|--------|--|-----------|-------|-----------|
| Bromobenzene | N.D. | 11.09 | 77.0 | 145.7 | 158.0 | 96.5 |
| + EIC (156.0) Scan 04JAN09.D ***NO DATA POINTS*** | | | 156.0, 77.0, 158.0 | | | |
|  | | |  | | | |
| 1,1,2-Tetrachloroethane | N.D. | 11.12 | 85.0 | 66.2 | | |
| + EIC (83.0) Scan 04JAN09.D | | | 83.0, 85.0 | | | |
|  | | |  | | | |
| 1,2,3-Trichloropropane | N.D. | 11.15 | 112.0 | 63.5 | | |
| + EIC (110.0) Scan 04JAN09.D | | | 110.0, 112.0 | | | |
|  | | |  | | | |
| 2-Chlorotoluene | N.D. | 11.29 | 91.0 | 282.3 | | |
| + EIC (126.0) Scan 04JAN09.D ***NO DATA POINTS*** | | | 126.0, 91.0 | | | |
|  | | |  | | | |

Quantitation Results Report (QT Reviewed)
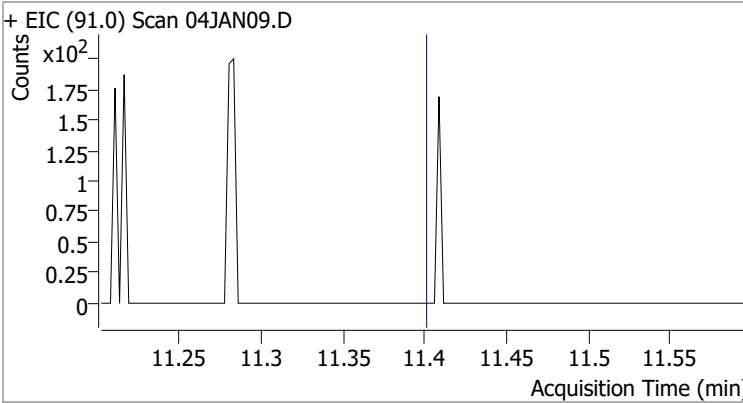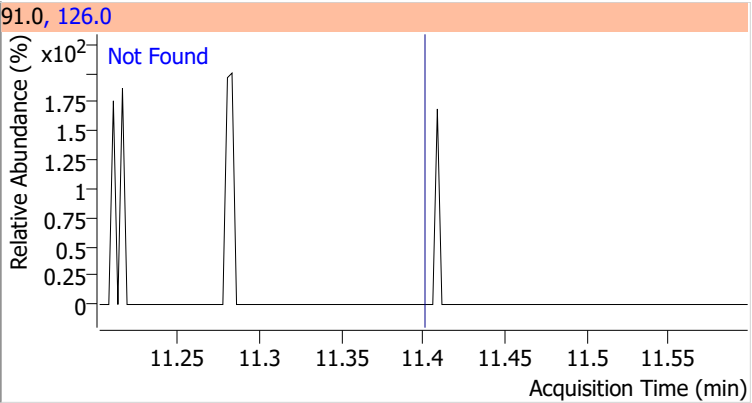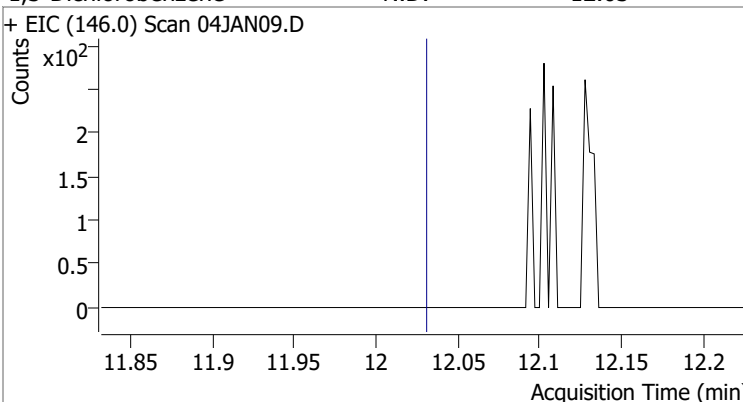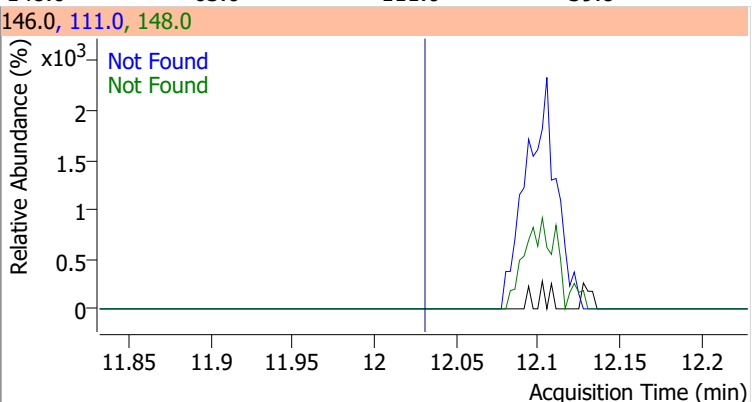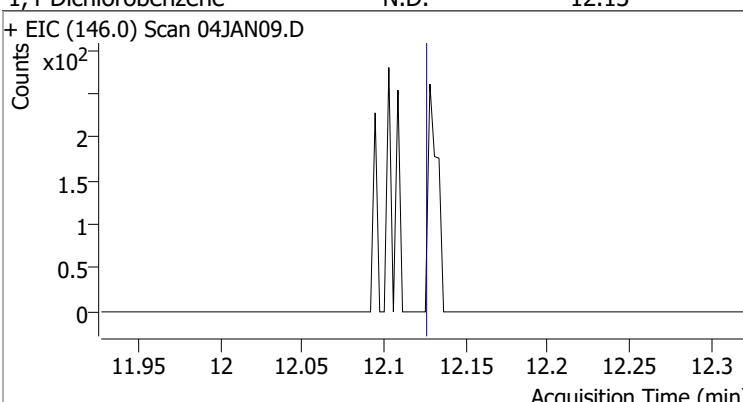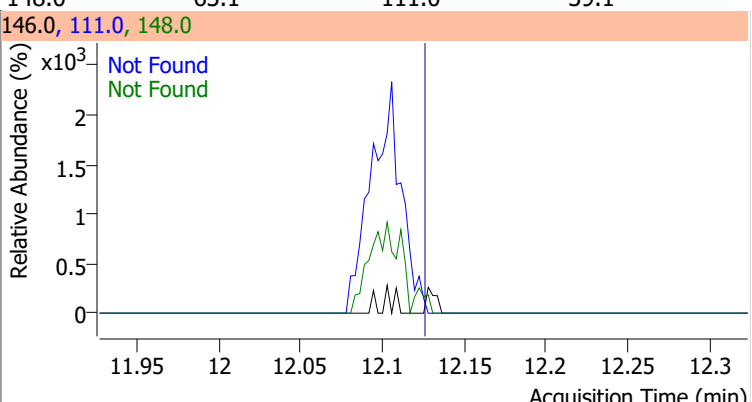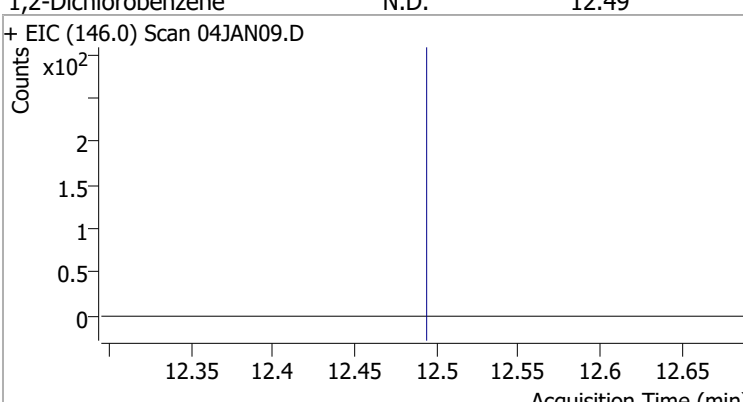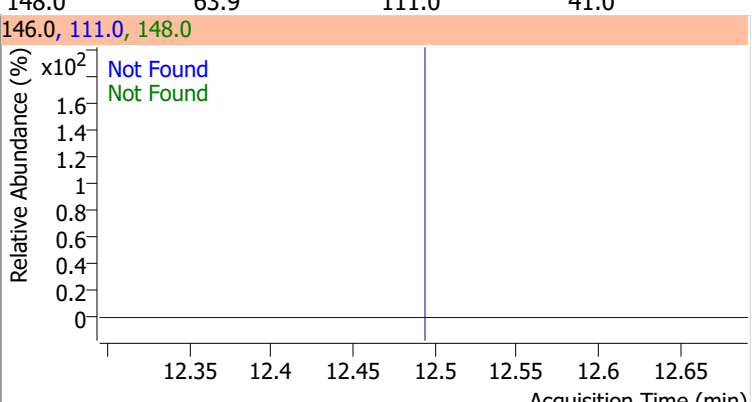
| Compound | Conc. | Exp RT | QIon | Exp Ratio | | |
|--|-------|--------|--|-----------|------|-----------|
| 4-Chlorotoluene | N.D. | 11.40 | 126.0 | 31.7 | | |
| + EIC (91.0) Scan 04JAN09.D | | | 91.0, 126.0 | | | |
|  | | |  | | | |
| 1,3-Dichlorobenzene | N.D. | 12.03 | 148.0 | 63.6 | QIon | Exp Ratio |
| + EIC (146.0) Scan 04JAN09.D | | | 146.0, 111.0, 148.0 | | | |
|  | | |  | | | |
| 1,4-Dichlorobenzene | N.D. | 12.13 | 148.0 | 63.1 | QIon | Exp Ratio |
| + EIC (146.0) Scan 04JAN09.D | | | 146.0, 111.0, 148.0 | | | |
|  | | |  | | | |
| 1,2-Dichlorobenzene | N.D. | 12.49 | 148.0 | 63.9 | QIon | Exp Ratio |
| + EIC (146.0) Scan 04JAN09.D | | | 146.0, 111.0, 148.0 | | | |
|  | | |  | | | |

Quantitation Results Report (QT Reviewed)

| | | | |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File | 04JAN10.D | Operator | MSC |
| Acq. Method | 5975CACQF.M | Acq. Date-Time | 1/4/2022 3:33:04 PM |
| Sample Name | ICAL010422_1 | Instrument | VOA5975C |
| Vial | 10 | Multiplier | 1.00 |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m | Comment | |
| Tune File | BFB_Atune3.u | Tune Date | 10/11/2021 4:02:00 PM |
| Batch Name | VG010422_8260B.batch.bin | Last Calib Update | 1/9/2022 8:59:52 PM |
| Ref Library | \\MASSHUNTER\Org\Library\NIST129K.l | | |







| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|------------------|-------|----------|
| Internal Standards | | | | | | |
| M Fluorobenzene | 6.621 | 96.0 | 770895 | 250.0000 | ng | -0.003 |
| M Chlorobenzene-d5 | 9.772 | 82.0 | 296081 | 250.0000 | ng | 0.000 |
| M 1,4-Dichlorobenzene-d4 | 12.100 | 152.0 | 227879 | 250.0000 | ng | 0.000 |
| System Monitoring Compounds | | | | | | |
| S Dibromofluoromethane | 5.851 | 113.0 | 2508 | 3.4533 | ng | m |
| Spiked Amount: 250.000 | Range: 80.0 - 119.0% | | | Recovery = 1.38% | * | |
| S 1,2-Dichloroethane-d4 | 6.233 | 67.0 | 923 | 2.9438 | ng | m |
| Spiked Amount: 250.000 | Range: 81.0 - 118.0% | | | Recovery = 1.18% | * | |
| S Toluene-d8 | 8.322 | 98.0 | 7777 | 2.7257 | ng | |
| Spiked Amount: 250.000 | Range: 89.0 - 112.0% | | | Recovery = 1.09% | * | |
| S p-Bromofluorobenzene | 10.951 | 95.0 | 2719 | 3.2569 | ng | -0.003 |
| Spiked Amount: 250.000 | Range: 85.0 - 114.0% | | | Recovery = 1.30% | * | |
| Target Compounds | | | | | | |
| T Dichlorodifluoromethane | 1.241 | 85.0 | 4353 | 4.3090 | ng | 99 |
| T Chloromethane | 1.406 | 50.0 | 7435 | 6.0637 | ng | 83 |
| T Vinyl chloride | 1.495 | 62.0 | 4274 | 3.8739 | ng | 94 |
| T Bromomethane | 1.796 | 96.0 | 1902 | 3.8547 | ng | m |
| T Chloroethane | 1.899 | 64.0 | 2178 | 3.9871 | ng | m |
| T Trichlorofluoromethane | 2.153 | 101.0 | 5030 | 3.6731 | ng | 91 |
| T 1,1-Dichloroethene | 2.700 | 96.0 | 2084 | 2.6839 | ng | m |
| T Methylene chloride | 3.324 | 49.0 | 4095 | 3.5774 | ng | 88 |
| T trans-1,2-Dichloroethene | 3.723 | 96.0 | 2146 | 2.7090 | ng | m |
| T Methyl tert-butyl ether (MTBE) | 3.759 | 73.0 | 2717 | 2.6532 | ng | m |
| T 1,1-Dichloroethane | 4.376 | 63.0 | 3892 | 2.6393 | ng | 91 |
| T 2,2-Dichloropropane | 5.196 | 77.0 | 2930 | 2.6520 | ng | m |
| T cis-1,2-Dichloroethene | 5.212 | 96.0 | 2376 | 2.9581 | ng | m |
| T Methyl ethyl ketone | 5.302 | 43.0 | 3035 | 27.8967 | ng | 85 |
| T Bromochloromethane | 5.522 | 128.0 | 807 | 2.4260 | ng | m |
| T Chloroform | 5.659 | 83.0 | 4248 | 2.8946 | ng | 97 |

Quantitation Results Report (QT Reviewed)

| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|-----------------------------|--------|-------|-------|--------|-------|----------|
| T 1,1,1-Trichloroethane | 5.831 | 97.0 | 3510 | 2.5521 | ng | 99 |
| T Carbon tetrachloride | 6.029 | 117.0 | 4342 | 3.2043 | ng | 77 |
| T 1,1-Dichloropropene | 6.041 | 75.0 | 2830 | 2.4201 | ng | 91 |
| T Benzene | 6.278 | 78.0 | 8408 | 2.7393 | ng | 98 |
| T 1,2-Dichloroethane | 6.322 | 62.0 | 2415 | 2.9090 | ng m | 96 |
| T Trichloroethene | 7.033 | 95.0 | 2372 | 2.6564 | ng m | 93 |
| T 1,2-Dichloropropane | 7.273 | 63.0 | 2148 | 2.7347 | ng | 93 |
| T Dibromomethane | 7.396 | 93.0 | 902 | 2.7162 | ng m | 88 |
| T Bromodichloromethane | 7.597 | 83.0 | 2536 | 2.7684 | ng | 98 |
| T cis-1,3-Dichloropropene | 8.054 | 75.0 | 2583 | 2.4939 | ng | 94 |
| T Toluene | 8.380 | 92.0 | 5039 | 2.6145 | ng | 93 |
| T trans-1,3-Dichloropropene | 8.634 | 75.0 | 1470 | 1.9942 | ng m | 83 |
| T 1,1,2-Trichloroethane | 8.810 | 83.0 | 960 | 2.5012 | ng m | 89 |
| T Tetrachloroethene | 8.932 | 163.8 | 2105 | 2.6772 | ng m | 95 |
| T 1,3-Dichloropropane | 8.977 | 76.0 | 2257 | 2.9881 | ng | 77 |
| T Chlorodibromomethane | 9.203 | 129.0 | 1468 | 2.4461 | ng m | 100 |
| T 1,2-Dibromoethane | 9.300 | 107.0 | 1299 | 3.0943 | ng m | 85 |
| T Chlorobenzene | 9.805 | 112.0 | 5771 | 2.7350 | ng | 100 |
| T 1,1,1,2-Tetrachloroethane | 9.889 | 131.0 | 1893 | 2.5659 | ng m | 98 |
| T Ethylbenzene | 9.920 | 91.0 | 9283 | 2.5367 | ng | 93 |
| T m+p-Xylenes | 10.045 | 106.0 | 7212 | 5.0712 | ng | 88 |
| T o-Xylene | 10.430 | 106.0 | 3330 | 2.6303 | ng # | 80 |
| T Styrene | 10.444 | 104.0 | 4408 | 2.1625 | ng | 98 |
| T Bromoform | 10.625 | 172.5 | 708 | 2.4287 | ng m | 87 |
| T Bromobenzene | 11.088 | 156.0 | 2024 | 2.7439 | ng m | 94 |
| T 1,1,2,2-Tetrachloroethane | 11.113 | 83.0 | 1142 | 2.6916 | ng m | 92 |
| T 1,2,3-Trichloropropane | 0.000 | | 0 | N.D. | | |
| T 2-Chlorotoluene | 11.292 | 126.0 | 1844 | 2.5124 | ng m | 97 |
| T 4-Chlorotoluene | 11.400 | 91.0 | 5419 | 2.2650 | ng | 96 |
| T 1,3-Dichlorobenzene | 12.033 | 146.0 | 3541 | 2.6327 | ng | 99 |
| T 1,4-Dichlorobenzene | 12.125 | 146.0 | 3787 | 2.7613 | ng | 90 |
| T 1,2-Dichlorobenzene | 12.499 | 146.0 | 3104 | 2.7307 | ng | 96 |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|-------|----|----------|-------|------|--------|-------|-------|
|----------|-------|----|----------|-------|------|--------|-------|-------|




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|-------|----|----------|-------|------|--------|-------|-------|
|----------|-------|----|----------|-------|------|--------|-------|-------|



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|-------|----|----------|-------|------|--------|-------|-------|
|----------|-------|----|----------|-------|------|--------|-------|-------|




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|-------|----|----------|-------|------|--------|-------|-------|
|----------|-------|----|----------|-------|------|--------|-------|-------|




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------------|--------|------|----------|----------|------|--------|-------|-------|
| trans-1,2-Dichloroethene | 2.7090 | 3.72 | 0.01 | 2146 (m) | 61.0 | 153.6 | 123.9 | 183.9 |
| | | | | | 98.0 | 66.5 | 35.7 | 95.7 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------------------|--------|------|----------|----------|------|--------|-------|-------|
| Methyl tert-butyl ether (MTBE) | 2.6532 | 3.76 | 0.01 | 2717 (m) | 57.0 | 19.6 | 0.0 | 54.6 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|--------|------|----------|-------|------|--------|-------|-------|
| 1,1-Dichloroethane | 2.6393 | 4.38 | 0.00 | 3892 | 65.0 | 34.6 | 2.1 | 62.1 |
| | | | | | 83.0 | 5.8 | 0.0 | 43.7 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|--------|------|----------|----------|------|--------|-------|-------|
| 2,2-Dichloropropane | 2.6520 | 5.20 | 0.00 | 2930 (m) | 41.0 | 76.7 | 36.5 | 96.5 |
| | | | | | 97.0 | 27.8 | 0.0 | 53.2 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|--------|------|----------|----------|------|--------|-------|-------|
| cis-1,2-Dichloroethene | 2.9581 | 5.21 | 0.00 | 2376 (m) | 61.0 | 174.2 | 137.2 | 197.2 |
| | | | | | 98.0 | 64.2 | 37.3 | 97.3 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|---------|------|----------|-------|------|--------|-------|-------|
| Methyl ethyl ketone | 27.8967 | 5.30 | 0.02 | 3035 | 72.0 | 14.3 | 0.0 | 51.3 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|--------|------|----------|---------|------|--------|-------|-------|
| Bromochloromethane | 2.4260 | 5.52 | 0.00 | 807 (m) | 49.0 | 208.8 | 152.9 | 212.9 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|--------|------|----------|-------|------|--------|-------|-------|
| Chloroform | 2.8946 | 5.66 | 0.01 | 4248 | 85.0 | 63.8 | 36.0 | 96.0 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|--------|------|----------|-------|------|--------|-------|-------|
| 1,1,1-Trichloroethane | 2.5521 | 5.83 | 0.00 | 3510 | 99.0 | 65.9 | 34.7 | 94.7 |
| | | | | | 61.0 | 48.6 | 18.1 | 78.1 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|--------|------|----------|----------|-------|--------|-------|-------|
| Dibromofluoromethane | 3.4533 | 5.85 | 0.01 | 2508 (m) | 191.5 | 19.1 | 0.0 | 53.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|--------|------|----------|-------|-------|--------|-------|-------|
| Carbon tetrachloride | 3.2043 | 6.03 | 0.01 | 4342 | 119.0 | 72.7 | 67.2 | 127.2 |
| | | | | | 121.0 | 20.8 | 0.1 | 60.1 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|--------|------|----------|-------|-------|--------|-------|-------|
| 1,1-Dichloropropene | 2.4201 | 6.04 | 0.00 | 2830 | 110.0 | 39.7 | 5.9 | 65.9 |
| | | | | | 77.0 | 37.2 | 0.1 | 60.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|--------|------|----------|---------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 2.9438 | 6.23 | 0.00 | 923 (m) | 65.0 | 208.6 | 166.5 | 226.5 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|--------|------|----------|-------|------|--------|-------|-------|
| Benzene | 2.7393 | 6.28 | 0.00 | 8408 | 77.0 | 22.4 | 0.0 | 53.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|--------|------|----------|----------|------|--------|-------|-------|
| 1,2-Dichloroethane | 2.9090 | 6.32 | 0.00 | 2415 (m) | 64.0 | 31.5 | 0.0 | 59.9 |
| | | | | | 98.0 | 4.9 | 0.0 | 37.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|--------|------|----------|----------|-------|--------|-------|-------|
| Trichloroethene | 2.6564 | 7.03 | 0.00 | 2372 (m) | 130.0 | 108.2 | 71.5 | 131.5 |
| | | | | | 97.0 | 69.9 | 34.1 | 94.1 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|--------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloropropane | 2.7347 | 7.27 | 0.00 | 2148 | 76.0 | 34.1 | 8.2 | 68.2 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------|--------|------|----------|---------|-------|--------|-------|-------|
| Dibromomethane | 2.7162 | 7.40 | 0.00 | 902 (m) | 173.5 | 111.2 | 83.7 | 143.7 |
| | | | | | 95.0 | 59.4 | 52.2 | 112.2 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|--------|------|----------|-------|-------|--------|-------|-------|
| Bromodichloromethane | 2.7684 | 7.60 | 0.01 | 2536 | 85.0 | 64.3 | 34.5 | 94.5 |
| | | | | | 127.0 | 5.1 | 0.0 | 39.6 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------------|--------|------|----------|-------|------|--------|-------|-------|
| cis-1,3-Dichloropropene | 2.4939 | 8.05 | -0.01 | 2583 | 39.0 | 56.5 | 23.3 | 83.3 |
| | | | | | 77.0 | 35.7 | 1.0 | 61.0 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|--------|------|----------|-------|-------|--------|-------|-------|
| Toluene-d8 | 2.7257 | 8.32 | 0.00 | 7777 | 100.0 | 67.9 | 34.4 | 94.4 |
| | | | | | 99.0 | 9.0 | 0.0 | 39.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|--------|------|----------|-------|------|--------|-------|-------|
| Toluene | 2.6145 | 8.38 | -0.01 | 5039 | 91.0 | 166.3 | 145.8 | 205.8 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|--------|------|----------|----------|------|--------|-------|-------|
| trans-1,3-Dichloropropene | 1.9942 | 8.63 | 0.00 | 1470 (m) | 39.0 | 68.0 | 23.4 | 83.4 |
| | | | | | 77.0 | 38.7 | 2.4 | 62.4 |















| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|--------|------|----------|---------|------|--------|-------|-------|
| 1,1,2-Trichloroethane | 2.5012 | 8.81 | -0.01 | 960 (m) | 97.0 | 114.4 | 84.6 | 144.6 |
| | | | | | 85.0 | 43.5 | 37.6 | 97.6 |







Quantitation Results Report (QT Reviewed)

| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|--------|------|----------|----------|----------------|---------------|--------------|----------------|
| Tetrachloroethene | 2.6772 | 8.93 | 0.00 | 2105 (m) | 165.8 129.0 | 135.5 95.3 | 98.6 61.5 | 158.6 121.5 |
| | | | | | | | | |
| 1,3-Dichloropropane | 2.9881 | 8.98 | 0.00 | 2257 | 78.0 | 20.0 | 2.9 | 62.9 |
| | | | | | | | | |
| Chlorodibromomethane | 2.4461 | 9.20 | 0.00 | 1468 (m) | 127.0 | 77.7 | 48.0 | 108.0 |
| | | | | | | | | |
| 1,2-Dibromoethane | 3.0943 | 9.30 | -0.01 | 1299 (m) | 109.0 | 80.0 | 64.5 | 124.5 |
| | | | | | | | | |

Quantitation Results Report (QT Reviewed)

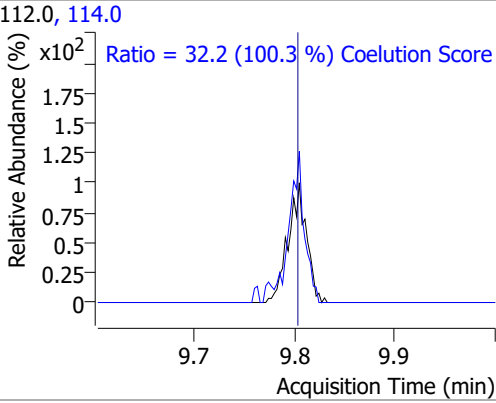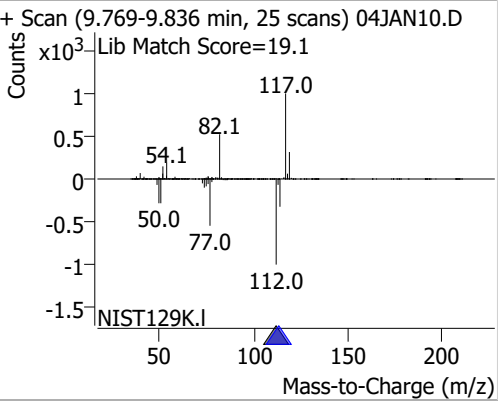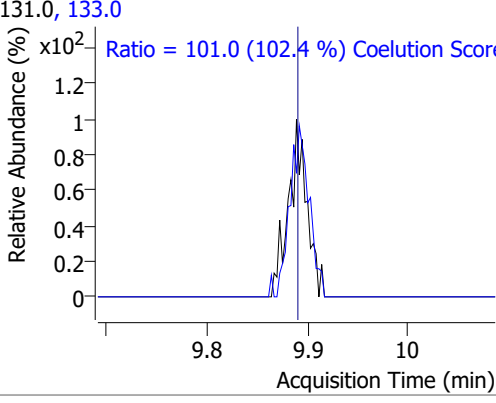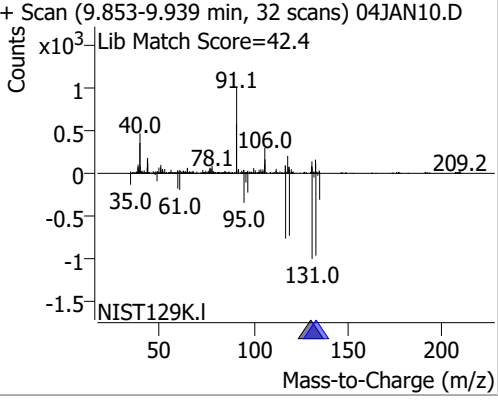
| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--|--|-------|---|----------|-------|--|-------|-------|
| Chlorobenzene | 2.7350 | 9.81 | 0.00 | 5771 | 114.0 | 32.2 | 2.1 | 62.1 |
| + EIC (112.0) Scan 04JAN10.D | | | 112.0, 114.0 | | | + Scan (9.769-9.836 min, 25 scans) 04JAN10.D | | |
|  |  | |  | | | | | |
| | | | Ratio = 32.2 (100.3 %) Coelution Score | | | Lib Match Score=19.1 | | |
| 1,1,1,2-Tetrachloroethane | 2.5659 | 9.89 | 0.00 | 1893 (m) | 133.0 | 101.0 | 68.6 | 128.6 |
| + EIC (131.0) Scan 04JAN10.D | | | 131.0, 133.0 | | | + Scan (9.853-9.939 min, 32 scans) 04JAN10.D | | |
|  |  | |  | | | | | |
| | | | Ratio = 101.0 (102.4 %) Coelution Score | | | Lib Match Score=42.4 | | |
| Ethylbenzene | 2.5367 | 9.92 | 0.00 | 9283 | 106.0 | 35.2 | 1.1 | 61.1 |
| + EIC (91.0) Scan 04JAN10.D | | | 91.0, 106.0 | | | + Scan (9.886-9.959 min, 27 scans) 04JAN10.D | | |
|  |  | |  | | | | | |
| | | | Ratio = 35.2 (113.0 %) Coelution Score | | | Lib Match Score=54.4 | | |
| m+p-Xylenes | 5.0712 | 10.05 | 0.01 | 7212 | 91.0 | 183.3 | 171.4 | 231.4 |
| + EIC (106.0) Scan 04JAN10.D | | | 106.0, 91.0 | | | + Scan (10.009-10.076 min, 25 scans) 04JAN10.D | | |
|  |  | |  | | | | | |
| | | | Ratio = 183.3 (91.0 %) Coelution Score | | | Lib Match Score=54.4 | | |

Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|--------|-------|----------|----------|-------|--------|-------|-------|
| Bromobenzene | 2.7439 | 11.09 | -0.01 | 2024 (m) | 77.0 | 134.0 | 115.7 | 175.7 |
| | | | | | 158.0 | 95.6 | 66.5 | 126.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|--------|-------|----------|----------|------|--------|-------|-------|
| 1,1,2,2-Tetrachloroethane | 2.6916 | 11.11 | 0.00 | 1142 (m) | 85.0 | 73.0 | 36.2 | 96.2 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|------------------------|-------|--------|-------|-----------|
| 1,2,3-Trichloropropane | N.D. | 11.15 | 112.0 | 63.5 |






| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|--------|-------|----------|----------|------|--------|-------|-------|
| 2-Chlorotoluene | 2.5124 | 11.29 | 0.00 | 1844 (m) | 91.0 | 288.1 | 252.3 | 312.3 |






Quantitation Results Report (QT Reviewed)




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|--------|-------|----------|-------|-------|--------|-------|-------|
| 4-Chlorotoluene | 2.2650 | 11.40 | 0.00 | 5419 | 126.0 | 33.9 | 1.7 | 61.7 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|--------|-------|----------|-------|-------|--------|-------|-------|
| 1,3-Dichlorobenzene | 2.6327 | 12.03 | 0.00 | 3541 | 148.0 | 63.6 | 33.6 | 93.6 |
| | | | | | 111.0 | 41.5 | 9.8 | 69.8 |






| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|--------|-------|----------|-------|-------|--------|-------|-------|
| 1,4-Dichlorobenzene | 2.7613 | 12.13 | 0.00 | 3787 | 148.0 | 66.5 | 33.1 | 93.1 |
| | | | | | 111.0 | 28.2 | 9.1 | 69.1 |



Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|--------|-------|----------|-------|-------|--------|-------|-------|
| 1,2-Dichlorobenzene | 2.7307 | 12.50 | 0.01 | 3104 | 148.0 | 61.0 | 33.9 | 93.9 |
| | | | | | 111.0 | 38.4 | 11.0 | 71.0 |



Quantitation Results Report (QT Reviewed)

Data File 04JAN11.D
 Acq. Method 5975CACQF.M
 Sample Name ICAL010422_2
 Vial 11
 DA Method File VOA5975C_8260B_SHT_DoD_L4_010422.m
 Tune File BFB_Atune3.u
 Batch Name VG010422_8260B.batch.bin
 Ref Library \\MASSHUNTER\Org\Library\NIST129K.I

Operator MSC
 Acq. Date-Time 1/4/2022 4:00:35 PM
 Instrument VOA5975C
 Multiplier 1.00
 Comment
 Tune Date 10/11/2021 4:02:00 PM
 Last Calib Update 1/9/2022 8:59:52 PM















| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|------------------|-------|----------|
| Internal Standards | | | | | | |
| M Fluorobenzene | 6.621 | 96.0 | 764419 | 250.0000 | ng | -0.003 |
| M Chlorobenzene-d5 | 9.774 | 82.0 | 296554 | 250.0000 | ng | 0.003 |
| M 1,4-Dichlorobenzene-d4 | 12.103 | 152.0 | 242142 | 250.0000 | ng | 0.003 |
| System Monitoring Compounds | | | | | | |
| S Dibromofluoromethane | 5.845 | 113.0 | 9074 | 12.6000 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 80.0 - 119.0% | | | Recovery = 5.04% | * | |
| S 1,2-Dichloroethane-d4 | 6.227 | 67.0 | 3938 | 12.6600 | ng | -0.006 |
| Spiked Amount: 250.000 | Range: 81.0 - 118.0% | | | Recovery = 5.06% | * | |
| S Toluene-d8 | 8.322 | 98.0 | 32318 | 11.3089 | ng | 0.003 |
| Spiked Amount: 250.000 | Range: 89.0 - 112.0% | | | Recovery = 4.52% | * | |
| S p-Bromofluorobenzene | 10.948 | 95.0 | 10059 | 11.3393 | ng | -0.006 |
| Spiked Amount: 250.000 | Range: 85.0 - 114.0% | | | Recovery = 4.54% | * | |
| Target Compounds | | | | | | |
| T Dichlorodifluoromethane | 1.244 | 85.0 | 12087 | 12.0663 | ng | 96 |
| T Chloromethane | 1.406 | 50.0 | 16859 | 13.8661 | ng | 100 |
| T Vinyl chloride | 1.498 | 62.0 | 13724 | 12.5446 | ng | 75 |
| T Bromomethane | 1.796 | 96.0 | 5893 | 12.0464 | ng | 97 |
| T Chloroethane | 1.897 | 64.0 | 8052 | 14.8670 | ng | m 98 |
| T Trichlorofluoromethane | 2.142 | 101.0 | 15431 | 11.3637 | ng | 95 |
| T 1,1-Dichloroethene | 2.700 | 96.0 | 9169 | 11.9081 | ng | 96 |
| T Methylene chloride | 3.338 | 49.0 | 17734 | 15.6236 | ng | 93 |
| T trans-1,2-Dichloroethene | 3.720 | 96.0 | 9821 | 12.5022 | ng | m 95 |
| T Methyl tert-butyl ether (MTBE) | 3.762 | 73.0 | 12515 | 12.3255 | ng | m 99 |
| T 1,1-Dichloroethane | 4.378 | 63.0 | 17642 | 12.0652 | ng | 94 |
| T 2,2-Dichloropropane | 5.196 | 77.0 | 13676 | 12.4820 | ng | 95 |
| T cis-1,2-Dichloroethene | 5.221 | 96.0 | 10008 | 12.5659 | ng | 95 |
| T Methyl ethyl ketone | 5.288 | 43.0 | 13167 | 122.0520 | ng | 95 |
| T Bromochloromethane | 5.516 | 128.0 | 4275 | 12.9568 | ng | 91 |
| T Chloroform | 5.656 | 83.0 | 19015 | 13.0668 | ng | 98 |

Quantitation Results Report (QT Reviewed)





| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|-----------------------------|--------|-------|-------|---------|-------|----------|
| T 1,1,1-Trichloroethane | 5.837 | 97.0 | 16623 | 12.1891 | ng | 97 |
| T Carbon tetrachloride | 6.021 | 117.0 | 16466 | 12.2545 | ng | 98 |
| T 1,1-Dichloropropene | 6.038 | 75.0 | 13149 | 11.3397 | ng | 94 |
| T Benzene | 6.278 | 78.0 | 37071 | 12.1801 | ng | 99 |
| T 1,2-Dichloroethane | 6.322 | 62.0 | 10202 | 12.3906 | ng | 92 |
| T Trichloroethene | 7.025 | 95.0 | 10442 | 11.6753 | ng | 94 |
| T 1,2-Dichloropropane | 7.270 | 63.0 | 9488 | 12.0602 | ng | 99 |
| T Dibromomethane | 7.399 | 93.0 | 4675 | 14.0619 | ng | 93 |
| T Bromodichloromethane | 7.585 | 83.0 | 11562 | 12.6014 | ng | 97 |
| T cis-1,3-Dichloropropene | 8.062 | 75.0 | 12525 | 12.0738 | ng | 94 |
| T Toluene | 8.388 | 92.0 | 21794 | 11.2899 | ng | 97 |
| T trans-1,3-Dichloropropene | 8.645 | 75.0 | 8683 | 11.7589 | ng | 98 |
| T 1,1,2-Trichloroethane | 8.824 | 83.0 | 5090 | 13.2340 | ng | m 91 |
| T Tetrachloroethene | 8.935 | 163.8 | 9238 | 11.7302 | ng | 99 |
| T 1,3-Dichloropropane | 8.985 | 76.0 | 8967 | 11.8526 | ng | 97 |
| T Chlorodibromomethane | 9.206 | 129.0 | 7718 | 12.8393 | ng | 97 |
| T 1,2-Dibromoethane | 9.300 | 107.0 | 5410 | 12.8640 | ng | 100 |
| T Chlorobenzene | 9.802 | 112.0 | 26461 | 12.5204 | ng | 99 |
| T 1,1,1,2-Tetrachloroethane | 9.889 | 131.0 | 9473 | 12.8225 | ng | 88 |
| T Ethylbenzene | 9.917 | 91.0 | 40470 | 11.0411 | ng | 99 |
| T m+p-Xylenes | 10.037 | 106.0 | 31538 | 22.1410 | ng | 100 |
| T o-Xylene | 10.430 | 106.0 | 13519 | 10.6612 | ng | 92 |
| T Styrene | 10.449 | 104.0 | 23472 | 11.4968 | ng | 100 |
| T Bromoform | 10.625 | 172.5 | 3652 | 11.7860 | ng | 92 |
| T Bromobenzene | 11.096 | 156.0 | 9663 | 12.3310 | ng | 96 |
| T 1,1,2,2-Tetrachloroethane | 11.116 | 83.0 | 5793 | 12.8437 | ng | 99 |
| T 1,2,3-Trichloropropane | 11.144 | 110.0 | 1654 | 13.7084 | ng | m 99 |
| T 2-Chlorotoluene | 11.289 | 126.0 | 8731 | 11.1977 | ng | 94 |
| T 4-Chlorotoluene | 11.400 | 91.0 | 28532 | 11.2233 | ng | 100 |
| T 1,3-Dichlorobenzene | 12.036 | 146.0 | 16932 | 11.8473 | ng | 99 |
| T 1,4-Dichlorobenzene | 12.122 | 146.0 | 17438 | 11.9662 | ng | 94 |
| T 1,2-Dichlorobenzene | 12.493 | 146.0 | 14666 | 12.1423 | ng | 98 |

(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)

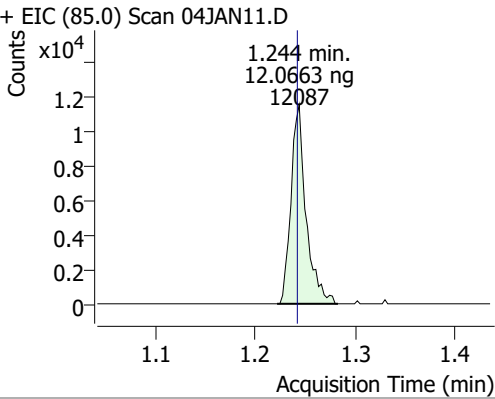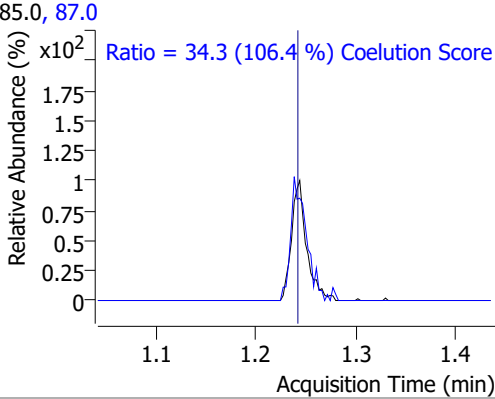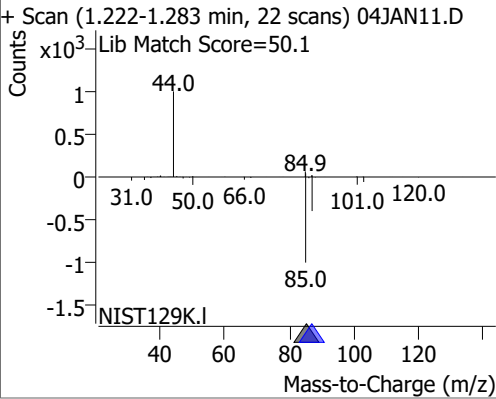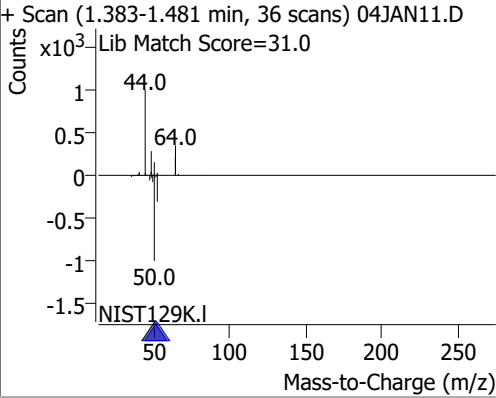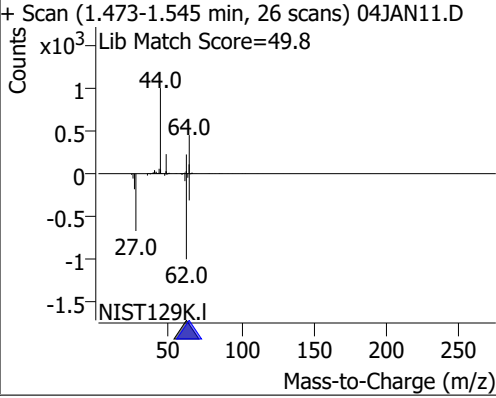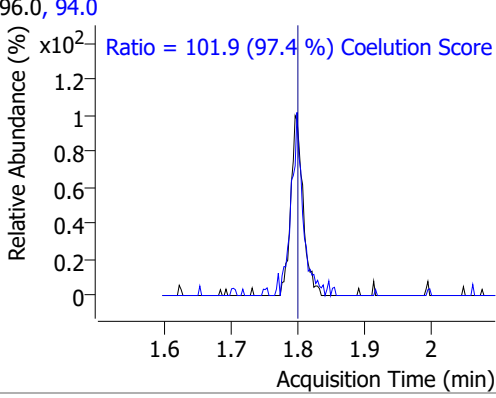
| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper | |
|--|--|------|--|-------|------|--|-------|-------|---|
| Dichlorodifluoromethane | 12.0663 | 1.24 | 0.00 | 12087 | 87.0 | 34.3 | 2.3 | 62.3 | |
| + EIC (85.0) Scan 04JAN11.D | | | 85.0, 87.0 | | | + Scan (1.222-1.283 min, 22 scans) 04JAN11.D | | | |
|  |  | | Ratio = 34.3 (106.4 %) Coelution Score | | | | | |  |
| Chloromethane | 13.8661 | 1.41 | 0.00 | 16859 | 52.0 | 32.0 | 2.1 | 62.1 | |
| + EIC (50.0) Scan 04JAN11.D | | | 50.0, 52.0 | | | + Scan (1.383-1.481 min, 36 scans) 04JAN11.D | | | |
|  |  | | Ratio = 32.0 (99.5 %) Coelution Score | | | | | |  |
| Vinyl chloride | 12.5446 | 1.50 | 0.00 | 13724 | 64.0 | 43.5 | 0.0 | 59.9 | |
| + EIC (62.0) Scan 04JAN11.D | | | 62.0, 64.0 | | | + Scan (1.473-1.545 min, 26 scans) 04JAN11.D | | | |
|  |  | | Ratio = 43.5 (145.5 %) Coelution Score | | | | | |  |
| Bromomethane | 12.0464 | 1.80 | 0.00 | 5893 | 94.0 | 101.9 | 74.6 | 134.6 | |
| + EIC (96.0) Scan 04JAN11.D | | | 96.0, 94.0 | | | + Scan (1.771-1.838 min, 25 scans) 04JAN11.D | | | |
|  |  | | Ratio = 101.9 (97.4 %) Coelution Score | | | | | |  |

Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------------|---------|------|----------|----------|------|--------|-------|-------|
| trans-1,2-Dichloroethene | 12.5022 | 3.72 | 0.00 | 9821 (m) | 61.0 | 146.7 | 123.9 | 183.9 |
| | | | | | 98.0 | 63.0 | 35.7 | 95.7 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------------------|---------|------|----------|-----------|------|--------|-------|-------|
| Methyl tert-butyl ether (MTBE) | 12.3255 | 3.76 | 0.01 | 12515 (m) | 57.0 | 24.3 | 0.0 | 54.6 |
| | | | | | | | | |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|---------|------|----------|-----------|------|--------|-------|-------|
| 1,1-Dichloroethane | 12.0652 | 4.38 | 0.00 | 17642 (m) | 65.0 | 35.8 | 2.1 | 62.1 |
| | | | | | 83.0 | 15.3 | 0.0 | 43.7 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|---------|------|----------|-------|------|--------|-------|-------|
| 2,2-Dichloropropane | 12.4820 | 5.20 | 0.00 | 13676 | 41.0 | 69.9 | 36.5 | 96.5 |
| | | | | | 97.0 | 27.3 | 0.0 | 53.2 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|---------|------|----------|-------|------|--------|-------|-------|
| cis-1,2-Dichloroethene | 12.5659 | 5.22 | 0.01 | 10008 | 61.0 | 158.3 | 137.2 | 197.2 |
| | | | | | 98.0 | 68.8 | 37.3 | 97.3 |







| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|-------|------|--------|-------|-------|
| Methyl ethyl ketone | 122.0520 | 5.29 | 0.01 | 13167 | 72.0 | 18.8 | 0.0 | 51.3 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|---------|------|----------|-------|------|--------|-------|-------|
| Bromochloromethane | 12.9568 | 5.52 | 0.00 | 4275 | 49.0 | 169.7 | 152.9 | 212.9 |




Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|---------|------|----------|-------|-------|--------|-------|-------|
| 1,1-Dichloropropene | 11.3397 | 6.04 | 0.00 | 13149 | 110.0 | 40.7 | 5.9 | 65.9 |
| | | | | | 77.0 | 31.6 | 0.1 | 60.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|---------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 12.6600 | 6.23 | -0.01 | 3938 | 65.0 | 220.5 | 166.5 | 226.5 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|---------|------|----------|-------|------|--------|-------|-------|
| Benzene | 12.1801 | 6.28 | 0.00 | 37071 | 77.0 | 23.8 | 0.0 | 53.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|---------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane | 12.3906 | 6.32 | 0.00 | 10202 | 64.0 | 35.2 | 0.0 | 59.9 |
| | | | | | 98.0 | 6.3 | 0.0 | 37.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|---------|------|----------|-------|-------|--------|-------|-------|
| Trichloroethene | 11.6753 | 7.02 | -0.01 | 10442 | 130.0 | 109.7 | 71.5 | 131.5 |
| | | | | | 97.0 | 66.1 | 34.1 | 94.1 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|---------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloropropane | 12.0602 | 7.27 | 0.00 | 9488 | 76.0 | 38.8 | 8.2 | 68.2 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------|---------|------|----------|-------|-------|--------|-------|-------|
| Dibromomethane | 14.0619 | 7.40 | 0.00 | 4675 | 173.5 | 106.3 | 83.7 | 143.7 |
| | | | | | 95.0 | 75.0 | 52.2 | 112.2 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|---------|------|----------|-------|-------|--------|-------|-------|
| Bromodichloromethane | 12.6014 | 7.59 | 0.00 | 11562 | 85.0 | 62.3 | 34.5 | 94.5 |
| | | | | | 127.0 | 8.2 | 0.0 | 39.6 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------------|---------|------|----------|-------|------|--------|-------|-------|
| cis-1,3-Dichloropropene | 12.0738 | 8.06 | 0.00 | 12525 | 39.0 | 57.8 | 23.3 | 83.3 |
| | | | | | 77.0 | 28.1 | 1.0 | 61.0 |






| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|---------|------|----------|-------|-------|--------|-------|-------|
| Toluene-d8 | 11.3089 | 8.32 | 0.00 | 32318 | 100.0 | 63.3 | 34.4 | 94.4 |
| | | | | | 99.0 | 8.9 | 0.0 | 39.6 |






Quantitation Results Report (QT Reviewed)




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|---------|------|----------|-------|------|--------|-------|-------|
| Toluene | 11.2899 | 8.39 | 0.00 | 21794 | 91.0 | 172.2 | 145.8 | 205.8 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|---------|------|----------|-------|--------------|--------------|-------------|--------------|
| trans-1,3-Dichloropropene | 11.7589 | 8.65 | 0.01 | 8683 | 39.0 77.0 | 53.4 35.5 | 23.4 2.4 | 83.4 62.4 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|---------|------|----------|----------|--------------|---------------|--------------|---------------|
| 1,1,2-Trichloroethane | 13.2340 | 8.82 | 0.01 | 5090 (m) | 97.0 85.0 | 105.6 59.6 | 84.6 37.6 | 144.6 97.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------|---------|------|----------|-------|----------------|---------------|--------------|----------------|
| Tetrachloroethene | 11.7302 | 8.94 | 0.00 | 9238 | 165.8 129.0 | 127.9 93.0 | 98.6 61.5 | 158.6 121.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|---------|------|----------|-------|------|--------|-------|-------|
| 1,3-Dichloropropane | 11.8526 | 8.99 | 0.01 | 8967 | 78.0 | 34.6 | 2.9 | 62.9 |







| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|---------|------|----------|-------|-------|--------|-------|-------|
| Chlorodibromomethane | 12.8393 | 9.21 | 0.00 | 7718 | 127.0 | 75.1 | 48.0 | 108.0 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------|---------|------|----------|-------|-------|--------|-------|-------|
| 1,2-Dibromoethane | 12.8640 | 9.30 | -0.01 | 5410 | 109.0 | 94.1 | 64.5 | 124.5 |




Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|---------|-------|----------|-------|------|--------|-------|-------|
| o-Xylene | 10.6612 | 10.43 | 0.00 | 13519 | 91.0 | 225.2 | 183.1 | 243.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|---------|-------|----------|-------|------|--------|-------|-------|
| Styrene | 11.4968 | 10.45 | 0.00 | 23472 | 78.0 | 49.5 | 19.6 | 79.6 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------|---------|-------|----------|-------|-------|--------|-------|-------|
| Bromoform | 11.7860 | 10.62 | 0.00 | 3652 | 170.5 | 55.5 | 22.1 | 82.1 |
| | | | | | 174.5 | 58.2 | 20.1 | 80.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|---------|-------|----------|-------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 11.3393 | 10.95 | -0.01 | 10059 | 174.0 | 98.3 | 61.7 | 121.7 |
| | | | | | 176.0 | 96.5 | 60.6 | 120.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|---------|-------|----------|-------|-------|--------|-------|-------|
| Bromobenzene | 12.3310 | 11.10 | 0.00 | 9663 | 77.0 | 140.9 | 115.7 | 175.7 |
| | | | | | 158.0 | 101.5 | 66.5 | 126.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|---------|-------|----------|-------|------|--------|-------|-------|
| 1,1,2,2-Tetrachloroethane | 12.8437 | 11.12 | 0.00 | 5793 | 85.0 | 67.4 | 36.2 | 96.2 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|---------|-------|----------|----------|-------|--------|-------|-------|
| 1,2,3-Trichloropropane | 13.7084 | 11.14 | 0.00 | 1654 (m) | 112.0 | 64.0 | 33.5 | 93.5 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|---------|-------|----------|-------|------|--------|-------|-------|
| 2-Chlorotoluene | 11.1977 | 11.29 | 0.00 | 8731 | 91.0 | 293.4 | 252.3 | 312.3 |






Quantitation Results Report (QT Reviewed)

| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------------|---------|-------|---------------------|-------|-------|--|-------|-------|
| 4-Chlorotoluene | 11.2233 | 11.40 | 0.00 | 28532 | 126.0 | 31.7 | 1.7 | 61.7 |
| + EIC (91.0) Scan 04JAN11.D | | | 91.0, 126.0 | | | + Scan (11.364-11.439 min, 28 scans) 04JAN11.D | | |
| | | | | | | | | |
| 1,3-Dichlorobenzene | 11.8473 | 12.04 | 0.01 | 16932 | 148.0 | 64.2 | 33.6 | 93.6 |
| + EIC (146.0) Scan 04JAN11.D | | | 146.0, 111.0, 148.0 | | | + Scan (12.000-12.067 min, 25 scans) 04JAN11.D | | |
| | | | | | | | | |
| 1,4-Dichlorobenzene | 11.9662 | 12.12 | 0.00 | 17438 | 148.0 | 70.5 | 33.1 | 93.1 |
| + EIC (146.0) Scan 04JAN11.D | | | 146.0, 111.0, 148.0 | | | + Scan (12.089-12.159 min, 25 scans) 04JAN11.D | | |
| | | | | | | | | |


Quantitation Results Report (QT Reviewed)

| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|---------|-------|----------|-------|-------|--------|-------|-------|
| 1,2-Dichlorobenzene | 12.1423 | 12.49 | 0.00 | 14666 | 148.0 | 66.1 | 33.9 | 93.9 |
| | | | | | 111.0 | 40.3 | 11.0 | 71.0 |
| | | | | | | | | |



Quantitation Results Report (QT Reviewed)

| | | | |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File | 04JAN12.D | Operator | MSC |
| Acq. Method | 5975CACQF.M | Acq. Date-Time | 1/4/2022 4:28:05 PM |
| Sample Name | ICAL010422_3 | Instrument | VOA5975C |
| Vial | 12 | Multiplier | 1.00 |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m | Comment | |
| Tune File | BFB_Atune3.u | Tune Date | 10/11/2021 4:02:00 PM |
| Batch Name | VG010422_8260B.batch.bin | Last Calib Update | 1/9/2022 8:59:52 PM |
| Ref Library | \\MASSHUNTER\Org\Library\NIST129K.I | | |











| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|-------------------|-------|----------|
| Internal Standards | | | | | | |
| M Fluorobenzene | 6.621 | 96.0 | 791270 | 250.0000 | ng | -0.003 |
| M Chlorobenzene-d5 | 9.775 | 82.0 | 301338 | 250.0000 | ng | 0.003 |
| M 1,4-Dichlorobenzene-d4 | 12.103 | 152.0 | 240335 | 250.0000 | ng | 0.003 |
| System Monitoring Compounds | | | | | | |
| S Dibromofluoromethane | 5.845 | 113.0 | 19100 | 25.6219 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 80.0 - 119.0% | | | Recovery = 10.25% | * | |
| S 1,2-Dichloroethane-d4 | 6.236 | 67.0 | 8284 | 25.7280 | ng | 0.003 |
| Spiked Amount: 250.000 | Range: 81.0 - 118.0% | | | Recovery = 10.29% | * | |
| S Toluene-d8 | 8.319 | 98.0 | 67673 | 23.3046 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 89.0 - 112.0% | | | Recovery = 9.32% | * | |
| S p-Bromofluorobenzene | 10.951 | 95.0 | 22267 | 25.2899 | ng | -0.003 |
| Spiked Amount: 250.000 | Range: 85.0 - 114.0% | | | Recovery = 10.12% | * | |
| Target Compounds | | | | | | |
| T Dichlorodifluoromethane | 1.244 | 85.0 | 26627 | 25.6793 | ng | 99 |
| T Chloromethane | 1.406 | 50.0 | 33153 | 26.3422 | ng | 95 |
| T Vinyl chloride | 1.495 | 62.0 | 29046 | 25.6488 | ng | 80 |
| T Bromomethane | 1.796 | 96.0 | 13054 | 25.7793 | ng | 99 |
| T Chloroethane | 1.897 | 64.0 | 14646 | 26.1250 | ng | m 92 |
| T Trichlorofluoromethane | 2.142 | 101.0 | 37464 | 26.6531 | ng | 98 |
| T 1,1-Dichloroethene | 2.700 | 96.0 | 20631 | 25.8849 | ng | 93 |
| T Methylene chloride | 3.333 | 49.0 | 30908 | 26.3058 | ng | 100 |
| T trans-1,2-Dichloroethene | 3.712 | 96.0 | 20706 | 25.4641 | ng | 97 |
| T Methyl tert-butyl ether (MTBE) | 3.754 | 73.0 | 24218 | 23.0418 | ng | 92 |
| T 1,1-Dichloroethane | 4.379 | 63.0 | 38874 | 25.6835 | ng | 97 |
| T 2,2-Dichloropropane | 5.190 | 77.0 | 29793 | 26.2692 | ng | 100 |
| T cis-1,2-Dichloroethene | 5.212 | 96.0 | 20252 | 24.5653 | ng | 98 |
| T Methyl ethyl ketone | 5.282 | 43.0 | 26248 | 235.0504 | ng | 98 |
| T Bromochloromethane | 5.522 | 128.0 | 8688 | 25.4383 | ng | 98 |
| T Chloroform | 5.653 | 83.0 | 36413 | 24.1734 | ng | 97 |

Quantitation Results Report (QT Reviewed)

| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) | |
|-----------------------------|--------|-------|-------|---------|-------|----------|----|
| T 1,1,1-Trichloroethane | 5.826 | 97.0 | 35547 | 25.1809 | ng | 96 | |
| T Carbon tetrachloride | 6.024 | 117.0 | 34462 | 24.7773 | ng | 99 | |
| T 1,1-Dichloropropene | 6.038 | 75.0 | 29241 | 24.3617 | ng | 96 | |
| T Benzene | 6.278 | 78.0 | 74956 | 23.7919 | ng | 97 | |
| T 1,2-Dichloroethane | 6.322 | 62.0 | 19996 | 23.4616 | ng | 97 | |
| T Trichloroethene | 7.028 | 95.0 | 21946 | 24.1484 | ng | 98 | |
| T 1,2-Dichloropropane | 7.270 | 63.0 | 20077 | 25.1147 | ng | 98 | |
| T Dibromomethane | 7.393 | 93.0 | 8055 | 23.8439 | ng | 97 | |
| T Bromodichloromethane | 7.583 | 83.0 | 22743 | 24.3940 | ng | 98 | |
| T cis-1,3-Dichloropropene | 8.057 | 75.0 | 24511 | 23.2528 | ng | 97 | |
| T Toluene | 8.389 | 92.0 | 46355 | 23.6319 | ng | 99 | |
| T trans-1,3-Dichloropropene | 8.634 | 75.0 | 17850 | 23.7894 | ng | 97 | |
| T 1,1,2-Trichloroethane | 8.815 | 83.0 | 10099 | 25.8400 | ng | 95 | |
| T Tetrachloroethene | 8.935 | 163.8 | 20322 | 25.3948 | ng | 97 | |
| T 1,3-Dichloropropane | 8.983 | 76.0 | 18745 | 24.3839 | ng | 99 | |
| T Chlorodibromomethane | 9.197 | 129.0 | 14873 | 24.3492 | ng | 99 | |
| T 1,2-Dibromoethane | 9.309 | 107.0 | 10410 | 24.3601 | ng | 95 | |
| T Chlorobenzene | 9.802 | 112.0 | 53047 | 24.7015 | ng | 100 | |
| T 1,1,1,2-Tetrachloroethane | 9.889 | 131.0 | 18130 | 24.1509 | ng | 100 | |
| T Ethylbenzene | 9.917 | 91.0 | 88428 | 23.7421 | ng | 100 | |
| T m+p-Xylenes | 10.039 | 106.0 | 66267 | 45.7836 | ng | 98 | |
| T o-Xylene | 10.427 | 106.0 | 30463 | 23.6420 | ng | 98 | |
| T Styrene | 10.447 | 104.0 | 48569 | 23.4119 | ng | 97 | |
| T Bromoform | 10.625 | 172.5 | 7972 | 25.9212 | ng | 96 | |
| T Bromobenzene | 11.094 | 156.0 | 19259 | 24.7613 | ng | 94 | |
| T 1,1,2,2-Tetrachloroethane | 11.110 | 83.0 | 12440 | 27.7883 | ng | 93 | |
| T 1,2,3-Trichloropropane | 11.149 | 110.0 | 3200 | 26.7144 | ng | m | 96 |
| T 2-Chlorotoluene | 11.286 | 126.0 | 19390 | 25.0550 | ng | 94 | |
| T 4-Chlorotoluene | 11.400 | 91.0 | 61551 | 24.3936 | ng | 100 | |
| T 1,3-Dichlorobenzene | 12.033 | 146.0 | 36559 | 25.7725 | ng | 97 | |
| T 1,4-Dichlorobenzene | 12.125 | 146.0 | 36635 | 25.3284 | ng | 92 | |
| T 1,2-Dichlorobenzene | 12.488 | 146.0 | 29899 | 24.9402 | ng | 98 | |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)

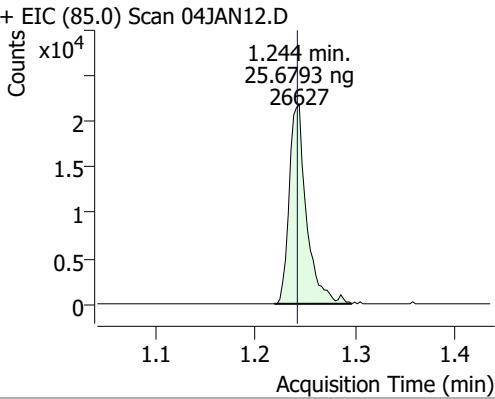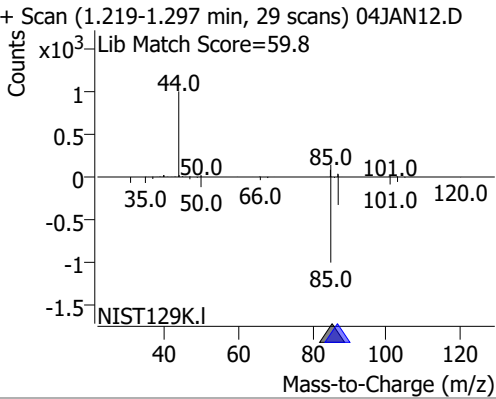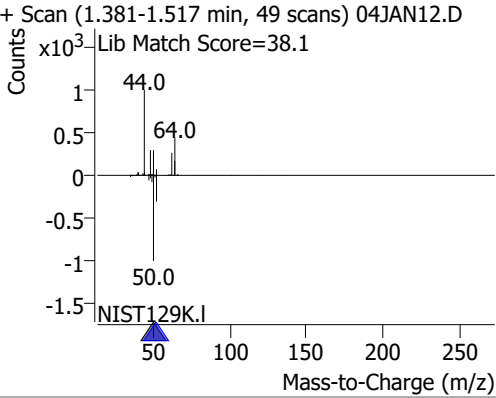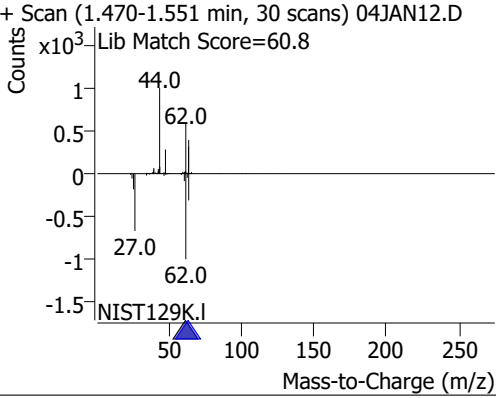
| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--|--|------|---|-------|------|--|-------|-------|
| Dichlorodifluoromethane | 25.6793 | 1.24 | 0.00 | 26627 | 87.0 | 31.7 | 2.3 | 62.3 |
| + EIC (85.0) Scan 04JAN12.D | | | 85.0, 87.0 | | | + Scan (1.219-1.297 min, 29 scans) 04JAN12.D | | |
|  | Ratio = 31.7 (98.4 %) Coelution Score = | |  | | | | | |
| Chloromethane | 26.3422 | 1.41 | 0.00 | 33153 | 52.0 | 29.4 | 2.1 | 62.1 |
| + EIC (50.0) Scan 04JAN12.D | | | 50.0, 52.0 | | | + Scan (1.381-1.517 min, 49 scans) 04JAN12.D | | |
|  | Ratio = 29.4 (91.6 %) Coelution Score = | |  | | | | | |
| Vinyl chloride | 25.6488 | 1.50 | 0.00 | 29046 | 64.0 | 40.6 | 0.0 | 59.9 |
| + EIC (62.0) Scan 04JAN12.D | | | 62.0, 64.0 | | | + Scan (1.470-1.551 min, 30 scans) 04JAN12.D | | |
|  | Ratio = 40.6 (135.6 %) Coelution Score = | |  | | | | | |
| Bromomethane | 25.7793 | 1.80 | 0.00 | 13054 | 94.0 | 103.7 | 74.6 | 134.6 |
| + EIC (96.0) Scan 04JAN12.D | | | 96.0, 94.0 | | | + Scan (1.766-1.838 min, 26 scans) 04JAN12.D | | |
|  | Ratio = 103.7 (99.1 %) Coelution Score = | |  | | | | | |

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|---------|------|----------|-----------|------|--------|-------|-------|
| Chloroethane | 26.1250 | 1.90 | 0.00 | 14646 (m) | 66.0 | 34.6 | 0.1 | 60.1 |




| | | | | | | | | |
|------------------------|---------|------|------|-------|-------|------|------|------|
| Trichlorofluoromethane | 26.6531 | 2.14 | 0.00 | 37464 | 103.0 | 62.6 | 34.2 | 94.2 |
|------------------------|---------|------|------|-------|-------|------|------|------|



| | | | | | | | | |
|--------------------|---------|------|------|-------|------|-------|-------|-------|
| 1,1-Dichloroethene | 25.8849 | 2.70 | 0.00 | 20631 | 61.0 | 169.5 | 150.3 | 210.3 |
| | | | | | 63.0 | 54.2 | 26.7 | 86.7 |




| | | | | | | | | |
|--------------------|---------|------|------|-------|------|------|------|------|
| Methylene chloride | 26.3058 | 3.33 | 0.00 | 30908 | 84.0 | 67.0 | 36.9 | 96.9 |
| | | | | | 86.0 | 44.2 | 14.3 | 74.3 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------------|---------|------|----------|-------|------|--------|-------|-------|
| trans-1,2-Dichloroethene | 25.4641 | 3.71 | -0.01 | 20706 | 61.0 | 152.1 | 123.9 | 183.9 |
| | | | | | 98.0 | 59.6 | 35.7 | 95.7 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------------------|---------|------|----------|-------|------|--------|-------|-------|
| Methyl tert-butyl ether (MTBE) | 23.0418 | 3.75 | 0.00 | 24218 | 57.0 | 28.7 | 0.0 | 54.6 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|---------|------|----------|-------|------|--------|-------|-------|
| 1,1-Dichloroethane | 25.6835 | 4.38 | 0.00 | 38874 | 65.0 | 33.1 | 2.1 | 62.1 |
| | | | | | 83.0 | 11.5 | 0.0 | 43.7 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|---------|------|----------|-------|------|--------|-------|-------|
| 2,2-Dichloropropane | 26.2692 | 5.19 | -0.01 | 29793 | 41.0 | 66.3 | 36.5 | 96.5 |
| | | | | | 97.0 | 23.4 | 0.0 | 53.2 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|---------|------|----------|-------|------|--------|-------|-------|
| cis-1,2-Dichloroethene | 24.5653 | 5.21 | 0.00 | 20252 | 61.0 | 168.5 | 137.2 | 197.2 |
| | | | | | 98.0 | 64.9 | 37.3 | 97.3 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|-------|------|--------|-------|-------|
| Methyl ethyl ketone | 235.0504 | 5.28 | 0.00 | 26248 | 72.0 | 20.4 | 0.0 | 51.3 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|---------|------|----------|-------|------|--------|-------|-------|
| Bromochloromethane | 25.4383 | 5.52 | 0.00 | 8688 | 49.0 | 186.0 | 152.9 | 212.9 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|---------|------|----------|-------|------|--------|-------|-------|
| Chloroform | 24.1734 | 5.65 | 0.00 | 36413 | 85.0 | 68.7 | 36.0 | 96.0 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|---------|------|----------|-------|------|--------|-------|-------|
| 1,1,1-Trichloroethane | 25.1809 | 5.83 | -0.01 | 35547 | 99.0 | 61.1 | 34.7 | 94.7 |
| | | | | | 61.0 | 45.9 | 18.1 | 78.1 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|---------|------|----------|-------|-------|--------|-------|-------|
| Dibromofluoromethane | 25.6219 | 5.85 | 0.00 | 19100 | 191.5 | 14.7 | 0.0 | 53.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|---------|------|----------|-------|-------|--------|-------|-------|
| Carbon tetrachloride | 24.7773 | 6.02 | 0.00 | 34462 | 119.0 | 97.0 | 67.2 | 127.2 |
| | | | | | 121.0 | 31.1 | 0.1 | 60.1 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|---------|------|----------|-------|-------|--------|-------|-------|
| 1,1-Dichloropropene | 24.3617 | 6.04 | 0.00 | 29241 | 110.0 | 33.6 | 5.9 | 65.9 |
| | | | | | 77.0 | 31.9 | 0.1 | 60.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|---------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 25.7280 | 6.24 | 0.00 | 8284 | 65.0 | 182.3 | 166.5 | 226.5 |
| | | | | | 77.0 | 31.9 | 0.1 | 60.1 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|---------|------|----------|-------|------|--------|-------|-------|
| Benzene | 23.7919 | 6.28 | 0.00 | 74956 | 77.0 | 25.0 | 0.0 | 53.5 |
| | | | | | 77.0 | 31.9 | 0.1 | 60.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|---------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane | 23.4616 | 6.32 | 0.00 | 19996 | 64.0 | 31.5 | 0.0 | 59.9 |
| | | | | | 98.0 | 8.3 | 0.0 | 37.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|---------|------|----------|-------|-------|--------|-------|-------|
| Trichloroethene | 24.1484 | 7.03 | 0.00 | 21946 | 130.0 | 102.4 | 71.5 | 131.5 |
| | | | | | 97.0 | 67.5 | 34.1 | 94.1 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|---------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloropropane | 25.1147 | 7.27 | 0.00 | 20077 | 76.0 | 37.1 | 8.2 | 68.2 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------|---------|------|----------|-------|-------|--------|-------|-------|
| Dibromomethane | 23.8439 | 7.39 | -0.01 | 8055 | 173.5 | 108.3 | 83.7 | 143.7 |
| | | | | | 95.0 | 81.9 | 52.2 | 112.2 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|---------|------|----------|-------|-------|--------|-------|-------|
| Bromodichloromethane | 24.3940 | 7.58 | 0.00 | 22743 | 85.0 | 66.3 | 34.5 | 94.5 |
| | | | | | 127.0 | 9.3 | 0.0 | 39.6 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------------|---------|------|----------|-------|------|--------|-------|-------|
| cis-1,3-Dichloropropene | 23.2528 | 8.06 | 0.00 | 24511 | 39.0 | 55.1 | 23.3 | 83.3 |
| | | | | | 77.0 | 33.2 | 1.0 | 61.0 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|---------|------|----------|-------|-------|--------|-------|-------|
| Toluene-d8 | 23.3046 | 8.32 | 0.00 | 67673 | 100.0 | 63.8 | 34.4 | 94.4 |
| | | | | | 99.0 | 9.1 | 0.0 | 39.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|---------|------|----------|-------|------|--------|-------|-------|
| Toluene | 23.6319 | 8.39 | 0.00 | 46355 | 91.0 | 174.6 | 145.8 | 205.8 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|---------|------|----------|-------|------|--------|-------|-------|
| trans-1,3-Dichloropropene | 23.7894 | 8.63 | 0.00 | 17850 | 39.0 | 55.9 | 23.4 | 83.4 |
| | | | | | 77.0 | 34.1 | 2.4 | 62.4 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|---------|------|----------|-------|------|--------|-------|-------|
| 1,1,2-Trichloroethane | 25.8400 | 8.82 | 0.00 | 10099 | 97.0 | 107.4 | 84.6 | 144.6 |
| | | | | | 85.0 | 66.1 | 37.6 | 97.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------|---------|------|----------|-------|-------|--------|-------|-------|
| Tetrachloroethene | 25.3948 | 8.94 | 0.00 | 20322 | 165.8 | 123.7 | 98.6 | 158.6 |
| | | | | | 129.0 | 90.9 | 61.5 | 121.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|---------|------|----------|-------|------|--------|-------|-------|
| 1,3-Dichloropropane | 24.3839 | 8.98 | 0.00 | 18745 | 78.0 | 33.6 | 2.9 | 62.9 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|---------|------|----------|-------|-------|--------|-------|-------|
| Chlorodibromomethane | 24.3492 | 9.20 | -0.01 | 14873 | 127.0 | 78.7 | 48.0 | 108.0 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------|---------|------|----------|-------|-------|--------|-------|-------|
| 1,2-Dibromoethane | 24.3601 | 9.31 | 0.00 | 10410 | 109.0 | 89.3 | 64.5 | 124.5 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------------|---------|-------|---|-------|-------|---|-------|-------|
| Chlorobenzene | 24.7015 | 9.80 | 0.00 | 53047 | 114.0 | 32.0 | 2.1 | 62.1 |
| + EIC (112.0) Scan 04JAN12.D | | | 112.0, 114.0 | | | + Scan (9.763-9.864 min, 37 scans) 04JAN12.D | | |
| | | | Ratio = 32.0 (99.5 %) Coelution Score = | | | | | |
| 1,1,1,2-Tetrachloroethane | 24.1509 | 9.89 | 0.00 | 18130 | 133.0 | 98.8 | 68.6 | 128.6 |
| + EIC (131.0) Scan 04JAN12.D | | | 131.0, 133.0 | | | + Scan (9.855-9.939 min, 31 scans) 04JAN12.D | | |
| | | | Ratio = 98.8 (100.2 %) Coelution Score = | | | | | |
| Ethylbenzene | 23.7421 | 9.92 | 0.00 | 88428 | 106.0 | 31.1 | 1.1 | 61.1 |
| + EIC (91.0) Scan 04JAN12.D | | | 91.0, 106.0 | | | + Scan (9.878-9.984 min, 39 scans) 04JAN12.D | | |
| | | | Ratio = 31.1 (99.9 %) Coelution Score = | | | | | |
| m+p-Xylenes | 45.7836 | 10.04 | 0.00 | 66267 | 91.0 | 204.5 | 171.4 | 231.4 |
| + EIC (106.0) Scan 04JAN12.D | | | 106.0, 91.0 | | | + Scan (9.998-10.092 min, 35 scans) 04JAN12.D | | |
| | | | Ratio = 204.5 (101.6 %) Coelution Score = | | | | | |

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|---------|-------|----------|-------|------|--------|-------|-------|
| o-Xylene | 23.6420 | 10.43 | 0.00 | 30463 | 91.0 | 210.5 | 183.1 | 243.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|---------|-------|----------|-------|------|--------|-------|-------|
| Styrene | 23.4119 | 10.45 | 0.00 | 48569 | 78.0 | 51.8 | 19.6 | 79.6 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------|---------|-------|----------|-------|-------|--------|-------|-------|
| Bromoform | 25.9212 | 10.63 | 0.00 | 7972 | 170.5 | 47.6 | 22.1 | 82.1 |
| | | | | | 174.5 | 50.7 | 20.1 | 80.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|---------|-------|----------|-------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 25.2899 | 10.95 | 0.00 | 22267 | 174.0 | 96.1 | 61.7 | 121.7 |
| | | | | | 176.0 | 89.8 | 60.6 | 120.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|---------|-------|----------|-------|-------|--------|-------|-------|
| Bromobenzene | 24.7613 | 11.09 | 0.00 | 19259 | 77.0 | 151.0 | 115.7 | 175.7 |
| | | | | | 158.0 | 104.1 | 66.5 | 126.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|---------|-------|----------|-------|------|--------|-------|-------|
| 1,1,2,2-Tetrachloroethane | 27.7883 | 11.11 | -0.01 | 12440 | 85.0 | 60.9 | 36.2 | 96.2 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|---------|-------|----------|----------|-------|--------|-------|-------|
| 1,2,3-Trichloropropane | 26.7144 | 11.15 | 0.00 | 3200 (m) | 112.0 | 66.8 | 33.5 | 93.5 |






| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|---------|-------|----------|-------|------|--------|-------|-------|
| 2-Chlorotoluene | 25.0550 | 11.29 | -0.01 | 19390 | 91.0 | 270.4 | 252.3 | 312.3 |






Quantitation Results Report (QT Reviewed)




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|---------|-------|----------|-------|-------|--------|-------|-------|
| 4-Chlorotoluene | 24.3936 | 11.40 | 0.00 | 61551 | 126.0 | 31.8 | 1.7 | 61.7 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|---------|-------|----------|-------|-------|--------|-------|-------|
| 1,3-Dichlorobenzene | 25.7725 | 12.03 | 0.00 | 36559 | 148.0 | 61.3 | 33.6 | 93.6 |
| | | | | | 111.0 | 38.2 | 9.8 | 69.8 |






| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|---------|-------|----------|-------|-------|--------|-------|-------|
| 1,4-Dichlorobenzene | 25.3284 | 12.13 | 0.00 | 36635 | 148.0 | 67.6 | 33.1 | 93.1 |
| | | | | | 111.0 | 46.4 | 9.1 | 69.1 |




Quantitation Results Report (QT Reviewed)

| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|---------|-------|----------|-------|-------|--------|-------|-------|
| 1,2-Dichlorobenzene | 24.9402 | 12.49 | -0.01 | 29899 | 148.0 | 62.9 | 33.9 | 93.9 |
| | | | | | 111.0 | 42.3 | 11.0 | 71.0 |



Quantitation Results Report (QT Reviewed)

| | | | |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File | 04JAN13.D | Operator | MSC |
| Acq. Method | 5975CACQF.M | Acq. Date-Time | 1/4/2022 4:55:32 PM |
| Sample Name | ICAL010422_4 | Instrument | VOA5975C |
| Vial | 13 | Multiplier | 1.00 |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m | Comment | |
| Tune File | BFB_Atune3.u | Tune Date | 10/11/2021 4:02:00 PM |
| Batch Name | VG010422_8260B.batch.bin | Last Calib Update | 1/9/2022 8:59:52 PM |
| Ref Library | \\MASSHUNTER\Org\Library\NIST129K.I | | |















| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|-------------------|-------|----------|
| Internal Standards | | | | | | |
| M Fluorobenzene | 6.623 | 96.0 | 778120 | 250.0000 | ng | 0.000 |
| M Chlorobenzene-d5 | 9.774 | 82.0 | 300356 | 250.0000 | ng | 0.003 |
| M 1,4-Dichlorobenzene-d4 | 12.100 | 152.0 | 248636 | 250.0000 | ng | 0.000 |
| System Monitoring Compounds | | | | | | |
| S Dibromofluoromethane | 5.848 | 113.0 | 35309 | 48.1661 | ng | 0.003 |
| Spiked Amount: 250.000 | Range: 80.0 - 119.0% | | | Recovery = 19.27% | | * |
| S 1,2-Dichloroethane-d4 | 6.233 | 67.0 | 15238 | 48.1252 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 81.0 - 118.0% | | | Recovery = 19.25% | | * |
| S Toluene-d8 | 8.319 | 98.0 | 136453 | 47.1441 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 89.0 - 112.0% | | | Recovery = 18.86% | | * |
| S p-Bromofluorobenzene | 10.951 | 95.0 | 42506 | 46.6647 | ng | -0.003 |
| Spiked Amount: 250.000 | Range: 85.0 - 114.0% | | | Recovery = 18.67% | | * |
| Target Compounds | | | | | | |
| T Dichlorodifluoromethane | 1.241 | 85.0 | 50457 | 49.4835 | ng | 97 |
| T Chloromethane | 1.408 | 50.0 | 61632 | 49.7983 | ng | 99 |
| T Vinyl chloride | 1.495 | 62.0 | 54521 | 48.9580 | ng | 96 |
| T Bromomethane | 1.799 | 96.0 | 23699 | 47.5921 | ng | 100 |
| T Chloroethane | 1.897 | 64.0 | 25484 | 46.2243 | ng | 98 |
| T Trichlorofluoromethane | 2.145 | 101.0 | 68163 | 49.3128 | ng | 98 |
| T 1,1-Dichloroethene | 2.702 | 96.0 | 38253 | 48.8056 | ng | 100 |
| T Methylene chloride | 3.335 | 49.0 | 58282 | 50.4421 | ng | 99 |
| T trans-1,2-Dichloroethene | 3.717 | 96.0 | 39596 | 49.5178 | ng | 99 |
| T Methyl tert-butyl ether (MTBE) | 3.757 | 73.0 | 49126 | 47.5301 | ng | 100 |
| T 1,1-Dichloroethane | 4.381 | 63.0 | 73205 | 49.1828 | ng | 100 |
| T 2,2-Dichloropropane | 5.193 | 77.0 | 56189 | 50.3804 | ng | 100 |
| T cis-1,2-Dichloroethene | 5.209 | 96.0 | 39251 | 48.4154 | ng | 99 |
| T Methyl ethyl ketone | 5.285 | 43.0 | 52648 | 479.4296 | ng | 99 |
| T Bromochloromethane | 5.516 | 128.0 | 17338 | 51.6233 | ng | 96 |
| T Chloroform | 5.650 | 83.0 | 71403 | 48.2031 | ng | 99 |

Quantitation Results Report (QT Reviewed)





| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|-----------------------------|--------|-------|--------|---------|-------|----------|
| T 1,1,1-Trichloroethane | 5.834 | 97.0 | 67007 | 48.2688 | ng | 98 |
| T Carbon tetrachloride | 6.026 | 117.0 | 65313 | 47.7520 | ng | 98 |
| T 1,1-Dichloropropene | 6.035 | 75.0 | 56376 | 47.7627 | ng | 99 |
| T Benzene | 6.277 | 78.0 | 148727 | 48.0054 | ng | 100 |
| T 1,2-Dichloroethane | 6.325 | 62.0 | 41058 | 48.9880 | ng | 97 |
| T Trichloroethene | 7.030 | 95.0 | 42682 | 47.1189 | ng | 98 |
| T 1,2-Dichloropropane | 7.273 | 63.0 | 37870 | 47.5273 | ng | 96 |
| T Dibromomethane | 7.396 | 93.0 | 15989 | 47.4844 | ng | 97 |
| T Bromodichloromethane | 7.585 | 83.0 | 43900 | 47.2409 | ng | 97 |
| T cis-1,3-Dichloropropene | 8.057 | 75.0 | 48886 | 46.5283 | ng | 97 |
| T Toluene | 8.388 | 92.0 | 91915 | 47.0116 | ng | 100 |
| T trans-1,3-Dichloropropene | 8.639 | 75.0 | 35179 | 47.0378 | ng | 100 |
| T 1,1,2-Trichloroethane | 8.815 | 83.0 | 18884 | 48.4759 | ng | 99 |
| T Tetrachloroethene | 8.935 | 163.8 | 36925 | 46.2932 | ng | 97 |
| T 1,3-Dichloropropane | 8.980 | 76.0 | 37457 | 48.8841 | ng | 98 |
| T Chlorodibromomethane | 9.203 | 129.0 | 28153 | 46.2411 | ng | 99 |
| T 1,2-Dibromoethane | 9.303 | 107.0 | 21037 | 49.3889 | ng | 93 |
| T Chlorobenzene | 9.802 | 112.0 | 101452 | 47.3959 | ng | 99 |
| T 1,1,1,2-Tetrachloroethane | 9.889 | 131.0 | 35544 | 47.5029 | ng | 99 |
| T Ethylbenzene | 9.917 | 91.0 | 173769 | 46.8079 | ng | 99 |
| T m+p-Xylenes | 10.039 | 106.0 | 133498 | 92.5347 | ng | 98 |
| T o-Xylene | 10.430 | 106.0 | 61016 | 47.5086 | ng | 98 |
| T Styrene | 10.444 | 104.0 | 96576 | 46.7052 | ng | 100 |
| T Bromoform | 10.625 | 172.5 | 16073 | 50.5170 | ng | 96 |
| T Bromobenzene | 11.093 | 156.0 | 38282 | 47.5759 | ng | 98 |
| T 1,1,2,2-Tetrachloroethane | 11.105 | 83.0 | 22514 | 48.6124 | ng | 99 |
| T 1,2,3-Trichloropropane | 11.146 | 110.0 | 6096 | 49.1924 | ng | 97 |
| T 2-Chlorotoluene | 11.289 | 126.0 | 37987 | 47.4466 | ng | 99 |
| T 4-Chlorotoluene | 11.400 | 91.0 | 126308 | 48.3865 | ng | 100 |
| T 1,3-Dichlorobenzene | 12.033 | 146.0 | 69539 | 47.3853 | ng | 99 |
| T 1,4-Dichlorobenzene | 12.125 | 146.0 | 71841 | 48.0106 | ng | 97 |
| T 1,2-Dichlorobenzene | 12.491 | 146.0 | 60213 | 48.5498 | ng | 98 |

(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)

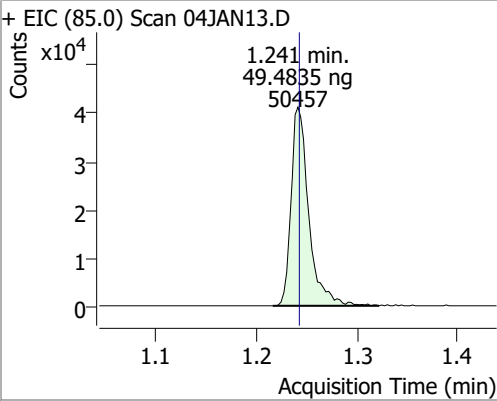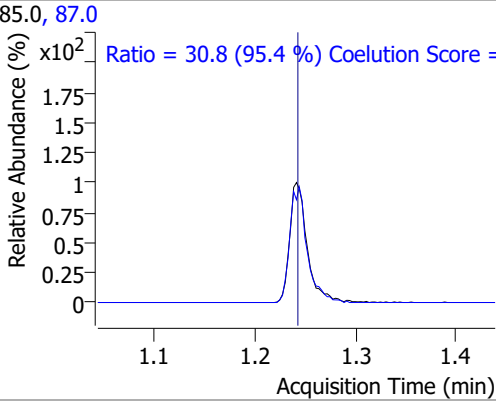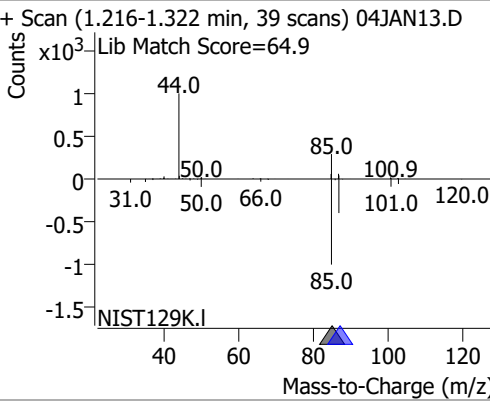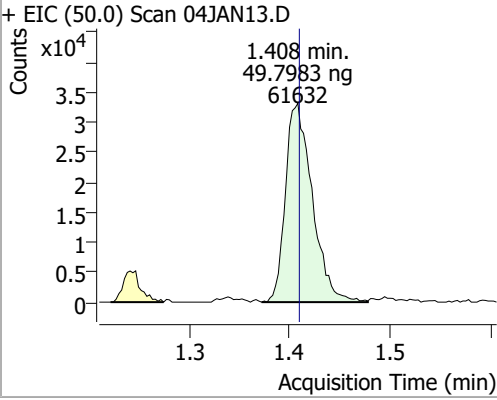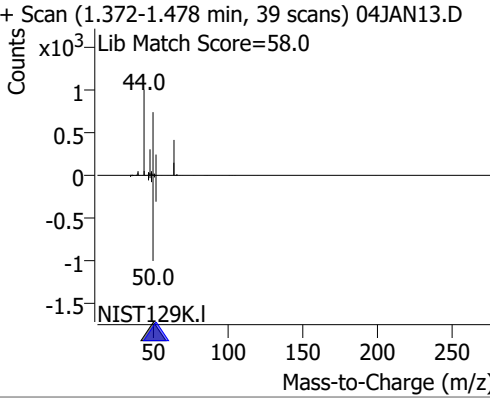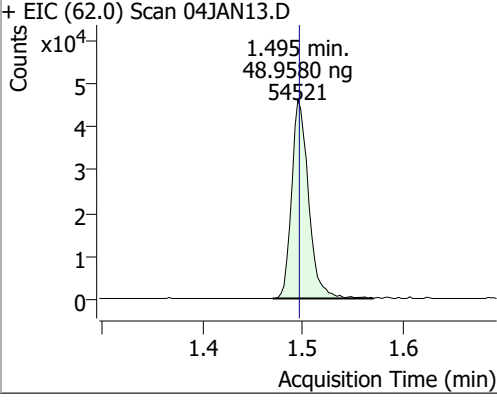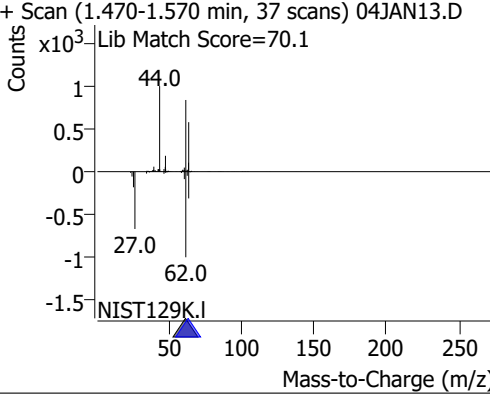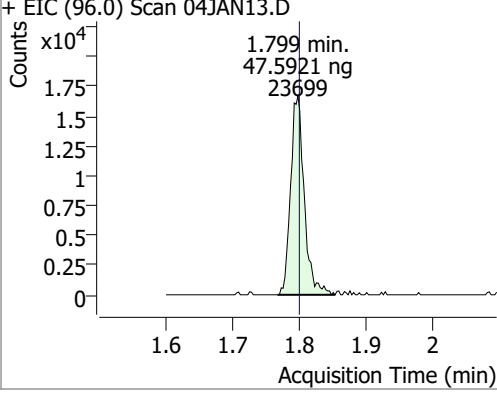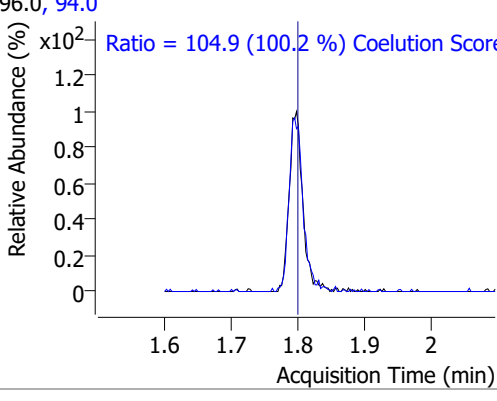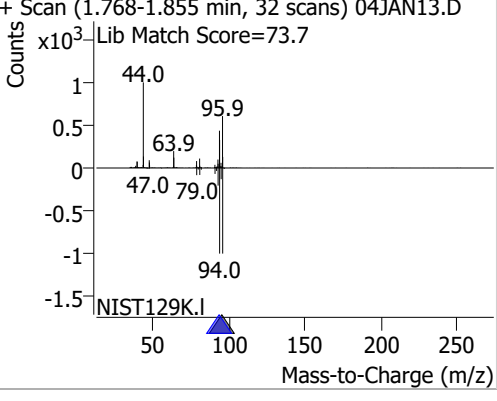
| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---|---------|------|--|-------|------|---|-------|-------|
| Dichlorodifluoromethane | 49.4835 | 1.24 | 0.00 | 50457 | 87.0 | 30.8 | 2.3 | 62.3 |
| + EIC (85.0) Scan 04JAN13.D  | | | 85.0, 87.0  | | | + Scan (1.216-1.322 min, 39 scans) 04JAN13.D Lib Match Score=64.9  | | |
| Chloromethane | 49.7983 | 1.41 | 0.00 | 61632 | 52.0 | 32.8 | 2.1 | 62.1 |
| + EIC (50.0) Scan 04JAN13.D  | | | 50.0, 52.0  | | | + Scan (1.372-1.478 min, 39 scans) 04JAN13.D Lib Match Score=58.0  | | |
| Vinyl chloride | 48.9580 | 1.49 | 0.00 | 54521 | 64.0 | 27.7 | 0.0 | 59.9 |
| + EIC (62.0) Scan 04JAN13.D  | | | 62.0, 64.0  | | | + Scan (1.470-1.570 min, 37 scans) 04JAN13.D Lib Match Score=70.1  | | |
| Bromomethane | 47.5921 | 1.80 | 0.00 | 23699 | 94.0 | 104.9 | 74.6 | 134.6 |
| + EIC (96.0) Scan 04JAN13.D  | | | 96.0, 94.0  | | | + Scan (1.768-1.855 min, 32 scans) 04JAN13.D Lib Match Score=73.7  | | |

Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------------|---------|------|----------|-------|------|--------|-------|-------|
| trans-1,2-Dichloroethene | 49.5178 | 3.72 | 0.00 | 39596 | 61.0 | 152.1 | 123.9 | 183.9 |
| | | | | | 98.0 | 65.3 | 35.7 | 95.7 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------------------|---------|------|----------|-------|------|--------|-------|-------|
| Methyl tert-butyl ether (MTBE) | 47.5301 | 3.76 | 0.00 | 49126 | 57.0 | 24.8 | 0.0 | 54.6 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|---------|------|----------|-------|------|--------|-------|-------|
| 1,1-Dichloroethane | 49.1828 | 4.38 | 0.00 | 73205 | 65.0 | 32.2 | 2.1 | 62.1 |
| | | | | | 83.0 | 13.7 | 0.0 | 43.7 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|---------|------|----------|-------|------|--------|-------|-------|
| 2,2-Dichloropropane | 50.3804 | 5.19 | 0.00 | 56189 | 41.0 | 66.6 | 36.5 | 96.5 |
| | | | | | 97.0 | 23.3 | 0.0 | 53.2 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|---------|------|----------|-------|------|--------|-------|-------|
| cis-1,2-Dichloroethene | 48.4154 | 5.21 | -0.01 | 39251 | 61.0 | 167.9 | 137.2 | 197.2 |
| | | | | | 98.0 | 66.0 | 37.3 | 97.3 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|-------|------|--------|-------|-------|
| Methyl ethyl ketone | 479.4296 | 5.28 | 0.00 | 52648 | 72.0 | 20.6 | 0.0 | 51.3 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|---------|------|----------|-------|------|--------|-------|-------|
| Bromochloromethane | 51.6233 | 5.52 | 0.00 | 17338 | 49.0 | 176.8 | 152.9 | 212.9 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|---------|------|----------|-------|------|--------|-------|-------|
| Chloroform | 48.2031 | 5.65 | 0.00 | 71403 | 85.0 | 65.5 | 36.0 | 96.0 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|---------|------|----------|-------|------|--------|-------|-------|
| 1,1,1-Trichloroethane | 48.2688 | 5.83 | 0.00 | 67007 | 99.0 | 65.2 | 34.7 | 94.7 |
| | | | | | 61.0 | 50.6 | 18.1 | 78.1 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|---------|------|----------|-------|-------|--------|-------|-------|
| Dibromofluoromethane | 48.1661 | 5.85 | 0.00 | 35309 | 191.5 | 22.5 | 0.0 | 53.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|---------|------|----------|-------|-------|--------|-------|-------|
| Carbon tetrachloride | 47.7520 | 6.03 | 0.00 | 65313 | 119.0 | 97.9 | 67.2 | 127.2 |
| | | | | | 121.0 | 32.5 | 0.1 | 60.1 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|---------|------|----------|-------|-------|--------|-------|-------|
| 1,1-Dichloropropene | 47.7627 | 6.03 | 0.00 | 56376 | 110.0 | 35.3 | 5.9 | 65.9 |
| | | | | | 77.0 | 31.1 | 0.1 | 60.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|---------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 48.1252 | 6.23 | 0.00 | 15238 | 65.0 | 202.3 | 166.5 | 226.5 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|---------|------|----------|--------|------|--------|-------|-------|
| Benzene | 48.0054 | 6.28 | 0.00 | 148727 | 77.0 | 23.7 | 0.0 | 53.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|---------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane | 48.9880 | 6.32 | 0.00 | 41058 | 64.0 | 30.9 | 0.0 | 59.9 |
| | | | | | 98.0 | 5.5 | 0.0 | 37.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|---------|------|----------|-------|-------|--------|-------|-------|
| Trichloroethene | 47.1189 | 7.03 | 0.00 | 42682 | 130.0 | 102.4 | 71.5 | 131.5 |
| | | | | | 97.0 | 66.2 | 34.1 | 94.1 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|---------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloropropane | 47.5273 | 7.27 | 0.00 | 37870 | 76.0 | 40.8 | 8.2 | 68.2 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------|---------|------|----------|-------|-------|--------|-------|-------|
| Dibromomethane | 47.4844 | 7.40 | 0.00 | 15989 | 173.5 | 117.0 | 83.7 | 143.7 |
| | | | | | 95.0 | 85.2 | 52.2 | 112.2 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|---------|------|----------|-------|-------|--------|-------|-------|
| Bromodichloromethane | 47.2409 | 7.59 | 0.00 | 43900 | 85.0 | 67.1 | 34.5 | 94.5 |
| | | | | | 127.0 | 10.1 | 0.0 | 39.6 |












| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------------|---------|------|----------|-------|------|--------|-------|-------|
| cis-1,3-Dichloropropene | 46.5283 | 8.06 | 0.00 | 48886 | 39.0 | 56.3 | 23.3 | 83.3 |
| | | | | | 77.0 | 30.9 | 1.0 | 61.0 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|---------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 47.1441 | 8.32 | 0.00 | 136453 | 100.0 | 63.8 | 34.4 | 94.4 |
| | | | | | 99.0 | 9.2 | 0.0 | 39.6 |




Quantitation Results Report (QT Reviewed)

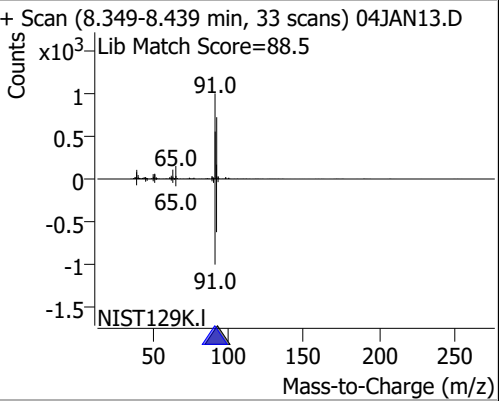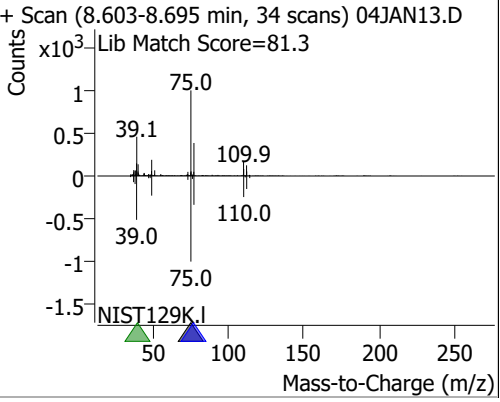
| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--|---------|------|--|-------|------|---|-------|-------|
| Toluene | 47.0116 | 8.39 | 0.00 | 91915 | 91.0 | 175.7 | 145.8 | 205.8 |
| + EIC (92.0) Scan 04JAN13.D | | | 92.0, 91.0 | | | + Scan (8.349-8.439 min, 33 scans) 04JAN13.D | | |
|  | | |  | | |  | | |
| trans-1,3-Dichloropropene | 47.0378 | 8.64 | 0.00 | 35179 | 39.0 | 53.4 | 23.4 | 83.4 |
| + EIC (75.0) Scan 04JAN13.D | | | 75.0, 77.0, 39.0 | | | + Scan (8.603-8.695 min, 34 scans) 04JAN13.D | | |
|  | | |  | | |  | | |
| 1,1,2-Trichloroethane | 48.4759 | 8.82 | 0.00 | 18884 | 97.0 | 115.3 | 84.6 | 144.6 |
| + EIC (83.0) Scan 04JAN13.D | | | 83.0, 97.0, 85.0 | | | + Scan (8.782-8.857 min, 28 scans) 04JAN13.D | | |
|  | | |  | | |  | | |

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------|---------|------|----------|-------|-------|--------|-------|-------|
| Tetrachloroethene | 46.2932 | 8.94 | 0.00 | 36925 | 165.8 | 132.7 | 98.6 | 158.6 |
| | | | | | 129.0 | 94.5 | 61.5 | 121.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|---------|------|----------|-------|------|--------|-------|-------|
| 1,3-Dichloropropane | 48.8841 | 8.98 | 0.00 | 37457 | 78.0 | 31.5 | 2.9 | 62.9 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|---------|------|----------|-------|-------|--------|-------|-------|
| Chlorodibromomethane | 46.2411 | 9.20 | 0.00 | 28153 | 127.0 | 77.4 | 48.0 | 108.0 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------|---------|------|----------|-------|-------|--------|-------|-------|
| 1,2-Dibromoethane | 49.3889 | 9.30 | 0.00 | 21037 | 109.0 | 88.2 | 64.5 | 124.5 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------------|---------|-------|--------------|--------|-------|--|-------|-------|
| Chlorobenzene | 47.3959 | 9.80 | 0.00 | 101452 | 114.0 | 32.8 | 2.1 | 62.1 |
| + EIC (112.0) Scan 04JAN13.D | | | 112.0, 114.0 | | | + Scan (9.760-9.880 min, 43 scans) 04JAN13.D | | |
| | | | | | | | | |
| 1,1,1,2-Tetrachloroethane | 47.5029 | 9.89 | 0.00 | 35544 | 133.0 | 97.3 | 68.6 | 128.6 |
| + EIC (131.0) Scan 04JAN13.D | | | 131.0, 133.0 | | | + Scan (9.852-9.936 min, 31 scans) 04JAN13.D | | |
| | | | | | | | | |
| Ethylbenzene | 46.8079 | 9.92 | 0.00 | 173769 | 106.0 | 30.6 | 1.1 | 61.1 |
| + EIC (91.0) Scan 04JAN13.D | | | 91.0, 106.0 | | | + Scan (9.878-9.986 min, 40 scans) 04JAN13.D | | |
| | | | | | | | | |
| m+p-Xylenes | 92.5347 | 10.04 | 0.00 | 133498 | 91.0 | 204.8 | 171.4 | 231.4 |
| + EIC (106.0) Scan 04JAN13.D | | | 106.0, 91.0 | | | + Scan (10.000-10.112 min, 41 scans) 04JAN13.D | | |
| | | | | | | | | |

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|---------|-------|----------|-------|------|--------|-------|-------|
| o-Xylene | 47.5086 | 10.43 | 0.00 | 61016 | 91.0 | 215.7 | 183.1 | 243.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|---------|-------|----------|-------|------|--------|-------|-------|
| Styrene | 46.7052 | 10.44 | 0.00 | 96576 | 78.0 | 49.7 | 19.6 | 79.6 |















| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------|---------|-------|----------|-------|-------|--------|-------|-------|
| Bromoform | 50.5170 | 10.62 | 0.00 | 16073 | 170.5 | 48.4 | 22.1 | 82.1 |
| | | | | | 174.5 | 47.8 | 20.1 | 80.1 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|---------|-------|----------|-------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 46.6647 | 10.95 | 0.00 | 42506 | 174.0 | 97.8 | 61.7 | 121.7 |
| | | | | | 176.0 | 93.2 | 60.6 | 120.6 |






Quantitation Results Report (QT Reviewed)

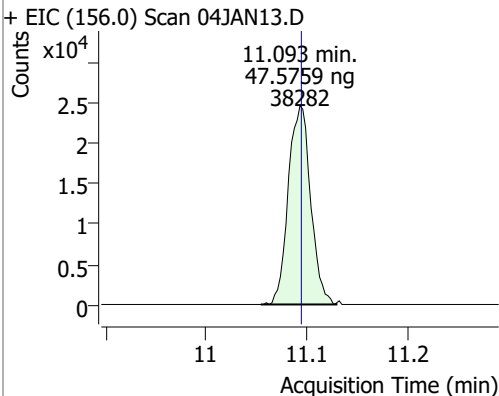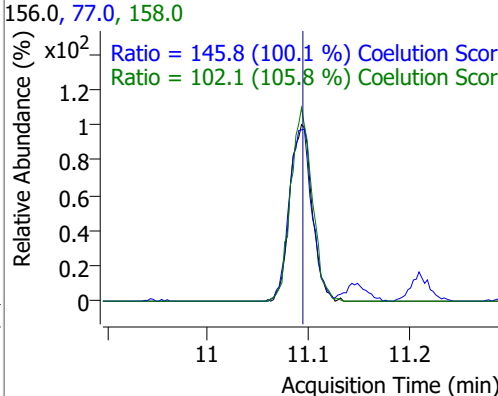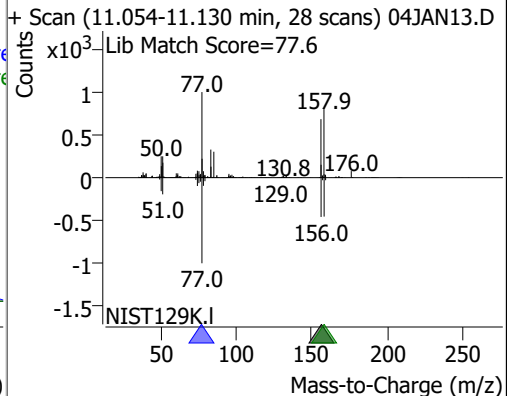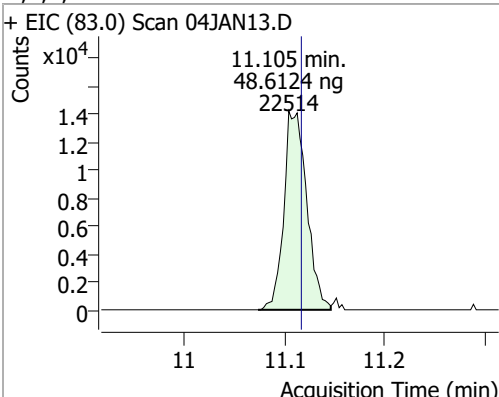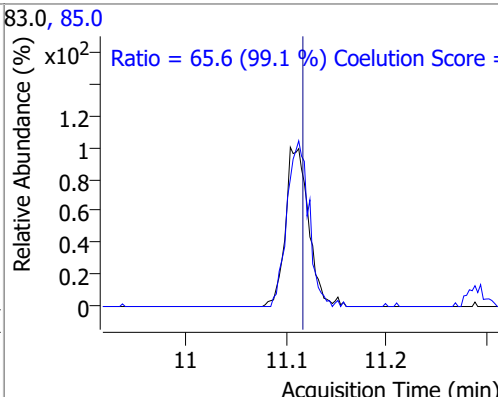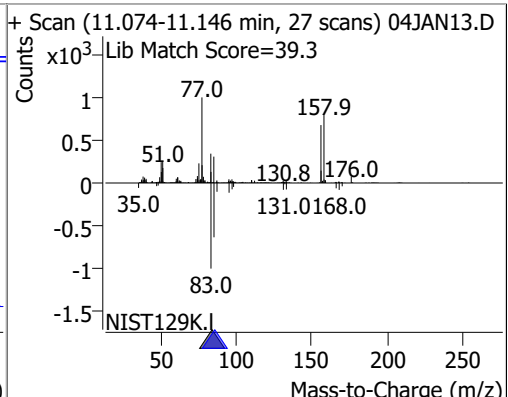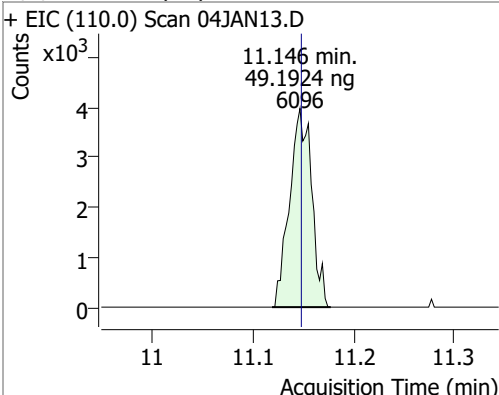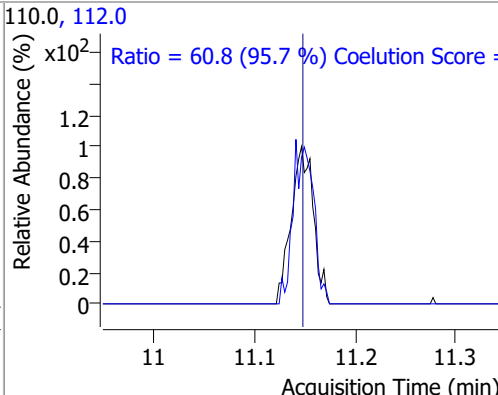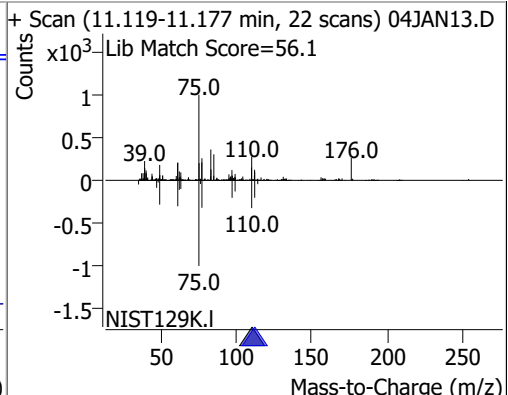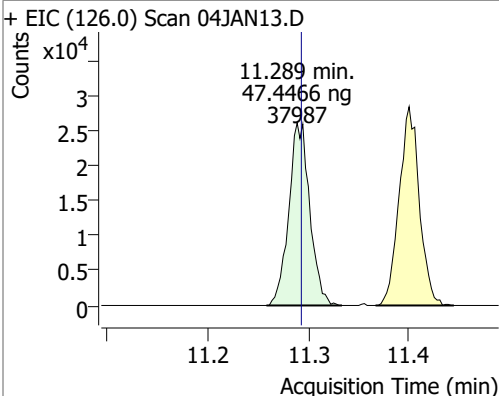
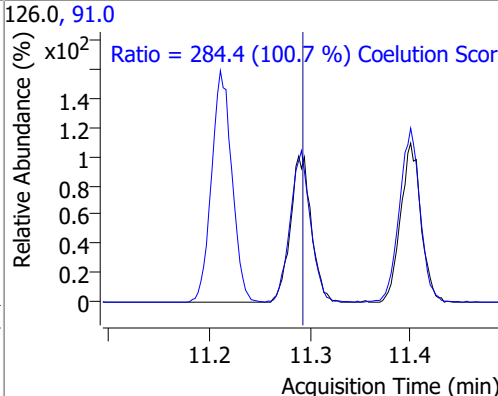
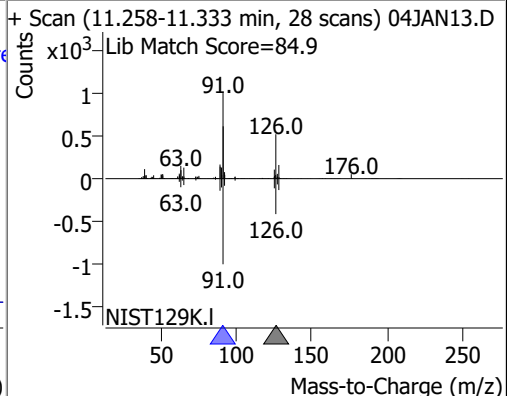
| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--|---------|-------|--|-------|---------------|---|---------------|----------------|
| Bromobenzene | 47.5759 | 11.09 | 0.00 | 38282 | 77.0 158.0 | 145.8 102.1 | 115.7 66.5 | 175.7 126.5 |
| + EIC (156.0) Scan 04JAN13.D | | | 156.0, 77.0, 158.0 | | | + Scan (11.054-11.130 min, 28 scans) 04JAN13.D | | |
|  | | |  | | |  | | |
| 1,1,2,2-Tetrachloroethane | 48.6124 | 11.10 | -0.01 | 22514 | 85.0 | 65.6 | 36.2 | 96.2 |
| + EIC (83.0) Scan 04JAN13.D | | | 83.0, 85.0 | | | + Scan (11.074-11.146 min, 27 scans) 04JAN13.D | | |
|  | | |  | | |  | | |
| 1,2,3-Trichloropropane | 49.1924 | 11.15 | 0.00 | 6096 | 112.0 | 60.8 | 33.5 | 93.5 |
| + EIC (110.0) Scan 04JAN13.D | | | 110.0, 112.0 | | | + Scan (11.119-11.177 min, 22 scans) 04JAN13.D | | |
|  | | |  | | |  | | |
| 2-Chlorotoluene | 47.4466 | 11.29 | 0.00 | 37987 | 91.0 | 284.4 | 252.3 | 312.3 |
| + EIC (126.0) Scan 04JAN13.D | | | 126.0, 91.0 | | | + Scan (11.258-11.333 min, 28 scans) 04JAN13.D | | |
|  | | |  | | |  | | |

Quantitation Results Report (QT Reviewed)




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|---------|-------|----------|--------|-------|--------|-------|-------|
| 4-Chlorotoluene | 48.3865 | 11.40 | 0.00 | 126308 | 126.0 | 31.6 | 1.7 | 61.7 |



| | | | | | | | | |
|---------------------|---------|-------|------|-------|-------|------|------|------|
| 1,3-Dichlorobenzene | 47.3853 | 12.03 | 0.00 | 69539 | 148.0 | 63.6 | 33.6 | 93.6 |
| | | | | | 111.0 | 37.9 | 9.8 | 69.8 |






| | | | | | | | | |
|---------------------|---------|-------|------|-------|-------|------|------|------|
| 1,4-Dichlorobenzene | 48.0106 | 12.13 | 0.00 | 71841 | 148.0 | 64.5 | 33.1 | 93.1 |
| | | | | | 111.0 | 41.8 | 9.1 | 69.1 |




Quantitation Results Report (QT Reviewed)

| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|---------|-------|----------|-------|-------|--------|-------|-------|
| 1,2-Dichlorobenzene | 48.5498 | 12.49 | 0.00 | 60213 | 148.0 | 61.9 | 33.9 | 93.9 |
| | | | | | 111.0 | 40.0 | 11.0 | 71.0 |



Quantitation Results Report (QT Reviewed)

| | | | |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File | 04JAN15.D | Operator | MSC |
| Acq. Method | 5975CACQF.M | Acq. Date-Time | 1/4/2022 5:50:25 PM |
| Sample Name | ICAL010422_5 | Instrument | VOA5975C |
| Vial | 15 | Multiplier | 1.00 |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m | Comment | |
| Tune File | BFB_Atune3.u | Tune Date | 10/11/2021 4:02:00 PM |
| Batch Name | VG010422_8260B.batch.bin | Last Calib Update | 1/9/2022 8:59:52 PM |
| Ref Library | \\MASSHUNTER\Org\Library\NIST129K.I | | |



| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|----------|----|------|-------|-------|-------|----------|
|----------|----|------|-------|-------|-------|----------|

Internal Standards

| | | | | | | |
|--------------------------|--------|-------|--------|----------|----|-------|
| M Fluorobenzene | 6.623 | 96.0 | 823488 | 250.0000 | ng | 0.000 |
| M Chlorobenzene-d5 | 9.772 | 82.0 | 306491 | 250.0000 | ng | 0.000 |
| M 1,4-Dichlorobenzene-d4 | 12.100 | 152.0 | 264477 | 250.0000 | ng | 0.000 |

System Monitoring Compounds

| | | | | | | |
|-------------------------|----------------------|-------|--------|-------------------|----|-------|
| S Dibromofluoromethane | 5.845 | 113.0 | 89307 | 115.1146 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 80.0 - 119.0% | | | Recovery = 46.05% | | * |
| S 1,2-Dichloroethane-d4 | 6.233 | 67.0 | 39086 | 116.6420 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 81.0 - 118.0% | | | Recovery = 46.66% | | * |
| S Toluene-d8 | 8.319 | 98.0 | 358186 | 121.2749 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 89.0 - 112.0% | | | Recovery = 48.51% | | * |
| S p-Bromofluorobenzene | 10.954 | 95.0 | 114269 | 117.9350 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 85.0 - 114.0% | | | Recovery = 47.17% | | * |

Target Compounds

| Compound | RT | QIon | Resp. | Conc. | Units | QValue |
|----------------------------------|-------|-------|--------|-----------|-------|--------|
| T Dichlorodifluoromethane | 1.241 | 85.0 | 137933 | 127.8193 | ng | 100 |
| T Chloromethane | 1.409 | 50.0 | 160604 | 122.6179 | ng | 100 |
| T Vinyl chloride | 1.495 | 62.0 | 148358 | 125.8809 | ng | 100 |
| T Bromomethane | 1.799 | 96.0 | 65163 | 123.6504 | ng | 100 |
| T Chloroethane | 1.894 | 64.0 | 71420 | 122.4086 | ng | 100 |
| T Trichlorofluoromethane | 2.142 | 101.0 | 188808 | 129.0687 | ng | 100 |
| T 1,1-Dichloroethene | 2.697 | 96.0 | 99438 | 119.8798 | ng | 100 |
| T Methylene chloride | 3.336 | 49.0 | 135271 | 110.6249 | ng | 100 |
| T trans-1,2-Dichloroethene | 3.718 | 96.0 | 100409 | 118.6511 | ng | 100 |
| T Methyl tert-butyl ether (MTBE) | 3.754 | 73.0 | 139068 | 127.1375 | ng | 100 |
| T 1,1-Dichloroethane | 4.378 | 63.0 | 186052 | 118.1125 | ng | 100 |
| T 2,2-Dichloropropane | 5.196 | 77.0 | 139656 | 118.3203 | ng | 100 |
| T cis-1,2-Dichloroethene | 5.215 | 96.0 | 100057 | 116.6190 | ng | 100 |
| T Methyl ethyl ketone | 5.282 | 43.0 | 134730 | 1159.3019 | ng | 100 |
| T Bromochloromethane | 5.519 | 128.0 | 41966 | 118.0683 | ng | 100 |
| T Chloroform | 5.653 | 83.0 | 179640 | 114.5912 | ng | 100 |


Quantitation Results Report (QT Reviewed)

| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|-----------------------------|--------|-------|--------|----------|-------|----------|
| T 1,1,1-Trichloroethane | 5.834 | 97.0 | 174206 | 118.5764 | ng | 100 |
| T Carbon tetrachloride | 6.024 | 117.0 | 172928 | 119.4667 | ng | 100 |
| T 1,1-Dichloropropene | 6.038 | 75.0 | 149649 | 119.8002 | ng | 100 |
| T Benzene | 6.278 | 78.0 | 383469 | 116.9553 | ng | 100 |
| T 1,2-Dichloroethane | 6.322 | 62.0 | 104855 | 118.2143 | ng | 100 |
| T Trichloroethene | 7.030 | 95.0 | 114123 | 123.4646 | ng | 100 |
| T 1,2-Dichloropropane | 7.270 | 63.0 | 99187 | 121.9890 | ng | 100 |
| T Dibromomethane | 7.399 | 93.0 | 40628 | 118.2425 | ng | 100 |
| T Bromodichloromethane | 7.585 | 83.0 | 115664 | 121.9749 | ng | 100 |
| T cis-1,3-Dichloropropene | 8.059 | 75.0 | 129419 | 120.7116 | ng | 100 |
| T Toluene | 8.389 | 92.0 | 244712 | 122.6571 | ng | 100 |
| T trans-1,3-Dichloropropene | 8.637 | 75.0 | 92719 | 121.4929 | ng | 100 |
| T 1,1,2-Trichloroethane | 8.818 | 83.0 | 46673 | 117.4130 | ng | 100 |
| T Tetrachloroethene | 8.935 | 163.8 | 97590 | 119.9003 | ng | 100 |
| T 1,3-Dichloropropane | 8.980 | 76.0 | 96183 | 123.0132 | ng | 100 |
| T Chlorodibromomethane | 9.206 | 129.0 | 75015 | 120.7454 | ng | 100 |
| T 1,2-Dibromoethane | 9.306 | 107.0 | 51827 | 119.2394 | ng | 100 |
| T Chlorobenzene | 9.802 | 112.0 | 263617 | 120.6903 | ng | 100 |
| T 1,1,1,2-Tetrachloroethane | 9.889 | 131.0 | 90898 | 119.0492 | ng | 100 |
| T Ethylbenzene | 9.920 | 91.0 | 464148 | 122.5243 | ng | 100 |
| T m+p-Xylenes | 10.039 | 106.0 | 368418 | 250.2587 | ng | 100 |
| T o-Xylene | 10.430 | 106.0 | 161509 | 123.2378 | ng | 100 |
| T Styrene | 10.447 | 104.0 | 268375 | 127.1910 | ng | 100 |
| T Bromoform | 10.628 | 172.5 | 39165 | 115.7218 | ng | 100 |
| T Bromobenzene | 11.094 | 156.0 | 102265 | 119.4801 | ng | 100 |
| T 1,1,2,2-Tetrachloroethane | 11.116 | 83.0 | 56958 | 115.6179 | ng | 100 |
| T 1,2,3-Trichloropropane | 11.147 | 110.0 | 14846 | 112.6261 | ng | 100 |
| T 2-Chlorotoluene | 11.292 | 126.0 | 102424 | 120.2675 | ng | 100 |
| T 4-Chlorotoluene | 11.400 | 91.0 | 336146 | 121.0591 | ng | 100 |
| T 1,3-Dichlorobenzene | 12.031 | 146.0 | 183404 | 117.4899 | ng | 100 |
| T 1,4-Dichlorobenzene | 12.125 | 146.0 | 189045 | 118.7699 | ng | 100 |
| T 1,2-Dichlorobenzene | 12.493 | 146.0 | 152284 | 115.4323 | ng | 100 |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------------|----------|------|----------|--------|------|--------|-------|-------|
| Dichlorodifluoromethane | 127.8193 | 1.24 | 0.00 | 137933 | 87.0 | 32.3 | 2.3 | 62.3 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------|----------|------|----------|--------|------|--------|-------|-------|
| Chloromethane | 122.6179 | 1.41 | 0.00 | 160604 | 52.0 | 32.1 | 2.1 | 62.1 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------|----------|------|----------|--------|------|--------|-------|-------|
| Vinyl chloride | 125.8809 | 1.50 | 0.00 | 148358 | 64.0 | 29.9 | 0.0 | 59.9 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|----------|------|----------|-------|------|--------|-------|-------|
| Bromomethane | 123.6504 | 1.80 | 0.00 | 65163 | 94.0 | 104.6 | 74.6 | 134.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|----------|------|----------|-------|------|--------|-------|-------|
| Chloroethane | 122.4086 | 1.89 | 0.00 | 71420 | 66.0 | 30.1 | 0.1 | 60.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Trichlorofluoromethane | 129.0687 | 2.14 | 0.00 | 188808 | 103.0 | 64.2 | 34.2 | 94.2 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,1-Dichloroethene | 119.8798 | 2.70 | 0.00 | 99438 | 61.0 | 180.3 | 150.3 | 210.3 |
| | | | | | 63.0 | 56.7 | 26.7 | 86.7 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| Methylene chloride | 110.6249 | 3.34 | 0.00 | 135271 | 84.0 | 66.9 | 36.9 | 96.9 |
| | | | | | 86.0 | 44.3 | 14.3 | 74.3 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------------|----------|------|----------|--------|------|--------|-------|-------|
| trans-1,2-Dichloroethene | 118.6511 | 3.72 | 0.00 | 100409 | 61.0 | 153.9 | 123.9 | 183.9 |
| | | | | | 98.0 | 65.7 | 35.7 | 95.7 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------------------|----------|------|----------|--------|------|--------|-------|-------|
| Methyl tert-butyl ether (MTBE) | 127.1375 | 3.75 | 0.00 | 139068 | 57.0 | 24.6 | 0.0 | 54.6 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1-Dichloroethane | 118.1125 | 4.38 | 0.00 | 186052 | 65.0 | 32.1 | 2.1 | 62.1 |
| | | | | | 83.0 | 13.7 | 0.0 | 43.7 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 2,2-Dichloropropane | 118.3203 | 5.20 | 0.00 | 139656 | 41.0 | 66.5 | 36.5 | 96.5 |
| | | | | | 97.0 | 23.2 | 0.0 | 53.2 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,2-Dichloroethene | 116.6190 | 5.22 | 0.00 | 100057 | 61.0 | 167.2 | 137.2 | 197.2 |
| | | | | | 98.0 | 67.3 | 37.3 | 97.3 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|-----------|------|----------|--------|------|--------|-------|-------|
| Methyl ethyl ketone | 1159.3019 | 5.28 | 0.00 | 134730 | 72.0 | 21.3 | 0.0 | 51.3 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|-------|------|--------|-------|-------|
| Bromochloromethane | 118.0683 | 5.52 | 0.00 | 41966 | 49.0 | 182.9 | 152.9 | 212.9 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|------|--------|-------|-------|
| Chloroform | 114.5912 | 5.65 | 0.00 | 179640 | 85.0 | 66.0 | 36.0 | 96.0 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|--------|--------------|--------------|--------------|--------------|
| 1,1,1-Trichloroethane | 118.5764 | 5.83 | 0.00 | 174206 | 99.0 61.0 | 64.7 48.1 | 34.7 18.1 | 94.7 78.1 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|-------|-------|--------|-------|-------|
| Dibromofluoromethane | 115.1146 | 5.85 | 0.00 | 89307 | 191.5 | 23.1 | 0.0 | 53.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|----------------|--------------|-------------|---------------|
| Carbon tetrachloride | 119.4667 | 6.02 | 0.00 | 172928 | 119.0 121.0 | 97.2 30.1 | 67.2 0.1 | 127.2 60.1 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|-------|--------|-------|-------|
| 1,1-Dichloropropene | 119.8002 | 6.04 | 0.00 | 149649 | 110.0 | 35.9 | 5.9 | 65.9 |
| | | | | | 77.0 | 30.1 | 0.1 | 60.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 116.6420 | 6.23 | 0.00 | 39086 | 65.0 | 196.5 | 166.5 | 226.5 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|------|----------|--------|------|--------|-------|-------|
| Benzene | 116.9553 | 6.28 | 0.00 | 383469 | 77.0 | 23.5 | 0.0 | 53.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloroethane | 118.2143 | 6.32 | 0.00 | 104855 | 64.0 | 29.9 | 0.0 | 59.9 |
| | | | | | 98.0 | 7.6 | 0.0 | 37.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|----------|------|----------|--------|-------|--------|-------|-------|
| Trichloroethene | 123.4646 | 7.03 | 0.00 | 114123 | 130.0 | 101.5 | 71.5 | 131.5 |
| | | | | | 97.0 | 64.1 | 34.1 | 94.1 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloropropane | 121.9890 | 7.27 | 0.00 | 99187 | 76.0 | 38.2 | 8.2 | 68.2 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------|----------|------|----------|-------|-------|--------|-------|-------|
| Dibromomethane | 118.2425 | 7.40 | 0.00 | 40628 | 173.5 | 113.7 | 83.7 | 143.7 |
| | | | | | 95.0 | 82.2 | 52.2 | 112.2 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Bromodichloromethane | 121.9749 | 7.59 | 0.00 | 115664 | 85.0 | 64.5 | 34.5 | 94.5 |
| | | | | | 127.0 | 9.6 | 0.0 | 39.6 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,3-Dichloropropene | 120.7116 | 8.06 | 0.00 | 129419 | 39.0 | 53.3 | 23.3 | 83.3 |
| | | | | | 77.0 | 31.0 | 1.0 | 61.0 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 121.2749 | 8.32 | 0.00 | 358186 | 100.0 | 64.4 | 34.4 | 94.4 |
| | | | | | 99.0 | 9.6 | 0.0 | 39.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|------|----------|--------|------|--------|-------|-------|
| Toluene | 122.6571 | 8.39 | 0.00 | 244712 | 91.0 | 175.8 | 145.8 | 205.8 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|----------|------|----------|-------|------|--------|-------|-------|
| trans-1,3-Dichloropropene | 121.4929 | 8.64 | 0.00 | 92719 | 39.0 | 53.4 | 23.4 | 83.4 |
| | | | | | 77.0 | 32.4 | 2.4 | 62.4 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,1,2-Trichloroethane | 117.4130 | 8.82 | 0.00 | 46673 | 97.0 | 114.6 | 84.6 | 144.6 |
| | | | | | 85.0 | 67.6 | 37.6 | 97.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------|----------|------|----------|-------|-------|--------|-------|-------|
| Tetrachloroethene | 119.9003 | 8.94 | 0.00 | 97590 | 165.8 | 128.6 | 98.6 | 158.6 |
| | | | | | 129.0 | 91.5 | 61.5 | 121.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,3-Dichloropropane | 123.0132 | 8.98 | 0.00 | 96183 | 78.0 | 32.9 | 2.9 | 62.9 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|-------|-------|--------|-------|-------|
| Chlorodibromomethane | 120.7454 | 9.21 | 0.00 | 75015 | 127.0 | 78.0 | 48.0 | 108.0 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------|----------|------|----------|-------|-------|--------|-------|-------|
| 1,2-Dibromoethane | 119.2394 | 9.31 | 0.00 | 51827 | 109.0 | 94.5 | 64.5 | 124.5 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------|----------|------|----------|--------|-------|--------|-------|-------|
| Chlorobenzene | 120.6903 | 9.80 | 0.00 | 263617 | 114.0 | 32.1 | 2.1 | 62.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|----------|------|----------|-------|-------|--------|-------|-------|
| 1,1,1,2-Tetrachloroethane | 119.0492 | 9.89 | 0.00 | 90898 | 133.0 | 98.6 | 68.6 | 128.6 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|----------|------|----------|--------|-------|--------|-------|-------|
| Ethylbenzene | 122.5243 | 9.92 | 0.00 | 464148 | 106.0 | 31.1 | 1.1 | 61.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------|----------|-------|----------|--------|------|--------|-------|-------|
| m+p-Xylenes | 250.2587 | 10.04 | 0.00 | 368418 | 91.0 | 201.4 | 171.4 | 231.4 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|-------|----------|--------|------|--------|-------|-------|
| o-Xylene | 123.2378 | 10.43 | 0.00 | 161509 | 91.0 | 213.1 | 183.1 | 243.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|-------|----------|--------|------|--------|-------|-------|
| Styrene | 127.1910 | 10.45 | 0.00 | 268375 | 78.0 | 49.6 | 19.6 | 79.6 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------|----------|-------|----------|-------|-------|--------|-------|-------|
| Bromoform | 115.7218 | 10.63 | 0.00 | 39165 | 170.5 | 52.1 | 22.1 | 82.1 |
| | | | | | 174.5 | 50.1 | 20.1 | 80.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 117.9350 | 10.95 | 0.00 | 114269 | 174.0 | 91.7 | 61.7 | 121.7 |
| | | | | | 176.0 | 90.6 | 60.6 | 120.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|----------|-------|----------|--------|-------|--------|-------|-------|
| Bromobenzene | 119.4801 | 11.09 | 0.00 | 102265 | 77.0 | 145.7 | 115.7 | 175.7 |
| | | | | | 158.0 | 96.5 | 66.5 | 126.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|----------|-------|----------|-------|------|--------|-------|-------|
| 1,1,2,2-Tetrachloroethane | 115.6179 | 11.12 | 0.00 | 56958 | 85.0 | 66.2 | 36.2 | 96.2 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|----------|-------|----------|-------|-------|--------|-------|-------|
| 1,2,3-Trichloropropane | 112.6261 | 11.15 | 0.00 | 14846 | 112.0 | 63.5 | 33.5 | 93.5 |






| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|----------|-------|----------|--------|------|--------|-------|-------|
| 2-Chlorotoluene | 120.2675 | 11.29 | 0.00 | 102424 | 91.0 | 282.3 | 252.3 | 312.3 |






Quantitation Results Report (QT Reviewed)




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 4-Chlorotoluene | 121.0591 | 11.40 | 0.00 | 336146 | 126.0 | 31.7 | 1.7 | 61.7 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,3-Dichlorobenzene | 117.4899 | 12.03 | 0.00 | 183404 | 148.0 | 63.6 | 33.6 | 93.6 |
| | | | | | 111.0 | 39.8 | 9.8 | 69.8 |






| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,4-Dichlorobenzene | 118.7699 | 12.13 | 0.00 | 189045 | 148.0 | 63.1 | 33.1 | 93.1 |
| | | | | | 111.0 | 39.1 | 9.1 | 69.1 |




Quantitation Results Report (QT Reviewed)

| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,2-Dichlorobenzene | 115.4323 | 12.49 | 0.00 | 152284 | 148.0 | 63.9 | 33.9 | 93.9 |
| | | | | | 111.0 | 41.0 | 11.0 | 71.0 |



Quantitation Results Report (QT Reviewed)

| | | | |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File | 04JAN17.D | Operator | MSC |
| Acq. Method | 5975CACQF.M | Acq. Date-Time | 1/4/2022 6:45:10 PM |
| Sample Name | ICAL010422_6 | Instrument | VOA5975C |
| Vial | 17 | Multiplier | 1.00 |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m | Comment | |
| Tune File | BFB_Atune3.u | Tune Date | 10/11/2021 4:02:00 PM |
| Batch Name | VG010422_8260B.batch.bin | Last Calib Update | 1/9/2022 8:59:52 PM |
| Ref Library | \\MASSHUNTER\Org\Library\NIST129K.I | | |



| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|----------|----|------|-------|-------|-------|----------|
|----------|----|------|-------|-------|-------|----------|

Internal Standards

| | | | | | | |
|--------------------------|--------|-------|--------|----------|----|--------|
| M Fluorobenzene | 6.620 | 96.0 | 836278 | 250.0000 | ng | -0.003 |
| M Chlorobenzene-d5 | 9.774 | 82.0 | 316399 | 250.0000 | ng | 0.003 |
| M 1,4-Dichlorobenzene-d4 | 12.100 | 152.0 | 266553 | 250.0000 | ng | 0.000 |

System Monitoring Compounds

| | | | | | | |
|-------------------------|----------------------|-------|--------|--------------------|----|--------|
| S Dibromofluoromethane | 5.845 | 113.0 | 204073 | 259.0223 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 80.0 - 119.0% | | | Recovery = 103.61% | | |
| S 1,2-Dichloroethane-d4 | 6.236 | 67.0 | 87876 | 258.2324 | ng | 0.003 |
| Spiked Amount: 250.000 | Range: 81.0 - 118.0% | | | Recovery = 103.29% | | |
| S Toluene-d8 | 8.319 | 98.0 | 823306 | 270.0265 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 89.0 - 112.0% | | | Recovery = 108.01% | | |
| S p-Bromofluorobenzene | 10.951 | 95.0 | 261042 | 267.3186 | ng | -0.003 |
| Spiked Amount: 250.000 | Range: 85.0 - 114.0% | | | Recovery = 106.93% | | |

Target Compounds

| Compound | RT | QIon | Resp. | Conc. | Units | QValue |
|----------------------------------|-------|-------|--------|-----------|-------|--------|
| T Dichlorodifluoromethane | 1.241 | 85.0 | 276334 | 252.1559 | ng | 99 |
| T Chloromethane | 1.408 | 50.0 | 319523 | 240.2183 | ng | 99 |
| T Vinyl chloride | 1.498 | 62.0 | 297604 | 248.6532 | ng | 86 |
| T Bromomethane | 1.799 | 96.0 | 134737 | 251.7606 | ng | 97 |
| T Chloroethane | 1.894 | 64.0 | 137312 | 231.7432 | ng | 98 |
| T Trichlorofluoromethane | 2.145 | 101.0 | 384837 | 259.0502 | ng | 98 |
| T 1,1-Dichloroethene | 2.702 | 96.0 | 217406 | 258.0903 | ng | 99 |
| T Methylene chloride | 3.333 | 49.0 | 292397 | 235.4657 | ng | 99 |
| T trans-1,2-Dichloroethene | 3.715 | 96.0 | 218855 | 254.6608 | ng | 99 |
| T Methyl tert-butyl ether (MTBE) | 3.751 | 73.0 | 287653 | 258.9535 | ng | 99 |
| T 1,1-Dichloroethane | 4.384 | 63.0 | 413408 | 258.4325 | ng | 99 |
| T 2,2-Dichloropropane | 5.190 | 77.0 | 303307 | 253.0397 | ng | 99 |
| T cis-1,2-Dichloroethene | 5.215 | 96.0 | 228170 | 261.8706 | ng | 96 |
| T Methyl ethyl ketone | 5.279 | 43.0 | 317271 | 2688.2474 | ng | 99 |
| T Bromochloromethane | 5.519 | 128.0 | 89178 | 247.0586 | ng | 95 |
| T Chloroform | 5.653 | 83.0 | 394946 | 248.0804 | ng | 99 |

Quantitation Results Report (QT Reviewed)

| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|-----------------------------|--------|-------|---------|----------|-------|----------|
| T 1,1,1-Trichloroethane | 5.831 | 97.0 | 386005 | 258.7228 | ng | 99 |
| T Carbon tetrachloride | 6.026 | 117.0 | 383485 | 260.8774 | ng | 99 |
| T 1,1-Dichloropropene | 6.038 | 75.0 | 335741 | 264.6638 | ng | 99 |
| T Benzene | 6.280 | 78.0 | 857534 | 257.5416 | ng | 100 |
| T 1,2-Dichloroethane | 6.322 | 62.0 | 226964 | 251.9675 | ng | 99 |
| T Trichloroethene | 7.030 | 95.0 | 250285 | 262.2931 | ng | 100 |
| T 1,2-Dichloropropane | 7.270 | 63.0 | 213800 | 254.7161 | ng | 100 |
| T Dibromomethane | 7.396 | 93.0 | 89483 | 252.2734 | ng | 97 |
| T Bromodichloromethane | 7.582 | 83.0 | 251805 | 257.2286 | ng | 100 |
| T cis-1,3-Dichloropropene | 8.057 | 75.0 | 293617 | 265.2863 | ng | 99 |
| T Toluene | 8.386 | 92.0 | 541945 | 263.1330 | ng | 100 |
| T trans-1,3-Dichloropropene | 8.639 | 75.0 | 207833 | 263.8027 | ng | 98 |
| T 1,1,2-Trichloroethane | 8.815 | 83.0 | 101888 | 248.2882 | ng | 99 |
| T Tetrachloroethene | 8.938 | 163.8 | 218245 | 259.7419 | ng | 98 |
| T 1,3-Dichloropropane | 8.980 | 76.0 | 212669 | 263.4754 | ng | 98 |
| T Chlorodibromomethane | 9.203 | 129.0 | 165695 | 258.3535 | ng | 100 |
| T 1,2-Dibromoethane | 9.306 | 107.0 | 115714 | 257.8887 | ng | 100 |
| T Chlorobenzene | 9.802 | 112.0 | 582326 | 258.2544 | ng | 100 |
| T 1,1,1,2-Tetrachloroethane | 9.891 | 131.0 | 200859 | 254.8274 | ng | 100 |
| T Ethylbenzene | 9.919 | 91.0 | 1043443 | 266.8193 | ng | 100 |
| T m+p-Xylenes | 10.039 | 106.0 | 825866 | 543.4262 | ng | 100 |
| T o-Xylene | 10.430 | 106.0 | 365914 | 270.4636 | ng | 100 |
| T Styrene | 10.446 | 104.0 | 605646 | 278.0455 | ng | 99 |
| T Bromoform | 10.628 | 172.5 | 87836 | 257.5099 | ng | 100 |
| T Bromobenzene | 11.093 | 156.0 | 227127 | 263.2944 | ng | 99 |
| T 1,1,2,2-Tetrachloroethane | 11.113 | 83.0 | 124205 | 250.1577 | ng | 97 |
| T 1,2,3-Trichloropropane | 11.152 | 110.0 | 33115 | 249.2635 | ng | 97 |
| T 2-Chlorotoluene | 11.291 | 126.0 | 229396 | 267.2616 | ng | 99 |
| T 4-Chlorotoluene | 11.400 | 91.0 | 748435 | 267.4409 | ng | 99 |
| T 1,3-Dichlorobenzene | 12.033 | 146.0 | 406895 | 258.6297 | ng | 99 |
| T 1,4-Dichlorobenzene | 12.122 | 146.0 | 408934 | 254.9170 | ng | 98 |
| T 1,2-Dichlorobenzene | 12.493 | 146.0 | 342576 | 257.6524 | ng | 99 |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------------|----------|------|------------|--------|------|--|-------|-------|
| Dichlorodifluoromethane | 252.1559 | 1.24 | 0.00 | 276334 | 87.0 | 31.6 | 2.3 | 62.3 |
| + EIC (85.0) Scan 04JAN17.D | | | 85.0, 87.0 | | | + Scan (1.216-1.344 min, 47 scans) 04JAN17.D | | |
| | | | | | | | | |
| Chloromethane | 240.2183 | 1.41 | 0.00 | 319523 | 52.0 | 32.9 | 2.1 | 62.1 |
| + EIC (50.0) Scan 04JAN17.D | | | 50.0, 52.0 | | | + Scan (1.367-1.537 min, 62 scans) 04JAN17.D | | |
| | | | | | | | | |
| Vinyl chloride | 248.6532 | 1.50 | 0.00 | 297604 | 64.0 | 37.7 | 0.0 | 59.9 |
| + EIC (62.0) Scan 04JAN17.D | | | 62.0, 64.0 | | | + Scan (1.467-1.615 min, 54 scans) 04JAN17.D | | |
| | | | | | | | | |
| Bromomethane | 251.7606 | 1.80 | 0.00 | 134737 | 94.0 | 107.5 | 74.6 | 134.6 |
| + EIC (96.0) Scan 04JAN17.D | | | 96.0, 94.0 | | | + Scan (1.760-1.919 min, 58 scans) 04JAN17.D | | |
| | | | | | | | | |

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|----------|------|----------|--------|------|--------|-------|-------|
| Chloroethane | 231.7432 | 1.89 | 0.00 | 137312 | 66.0 | 31.0 | 0.1 | 60.1 |




| | | | | | | | | |
|------------------------|----------|------|------|--------|-------|------|------|------|
| Trichlorofluoromethane | 259.0502 | 2.14 | 0.00 | 384837 | 103.0 | 65.6 | 34.2 | 94.2 |
|------------------------|----------|------|------|--------|-------|------|------|------|



| | | | | | | | | |
|--------------------|----------|------|------|--------|------|-------|-------|-------|
| 1,1-Dichloroethene | 258.0903 | 2.70 | 0.01 | 217406 | 61.0 | 181.2 | 150.3 | 210.3 |
| | | | | | 63.0 | 56.8 | 26.7 | 86.7 |




| | | | | | | | | |
|--------------------|----------|------|------|--------|------|------|------|------|
| Methylene chloride | 235.4657 | 3.33 | 0.00 | 292397 | 84.0 | 66.4 | 36.9 | 96.9 |
| | | | | | 86.0 | 42.7 | 14.3 | 74.3 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------------|----------|------|----------|--------|------|--------|-------|-------|
| trans-1,2-Dichloroethene | 254.6608 | 3.71 | 0.00 | 218855 | 61.0 | 153.9 | 123.9 | 183.9 |
| | | | | | 98.0 | 63.7 | 35.7 | 95.7 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------------------|----------|------|----------|--------|------|--------|-------|-------|
| Methyl tert-butyl ether (MTBE) | 258.9535 | 3.75 | 0.00 | 287653 | 57.0 | 25.3 | 0.0 | 54.6 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1-Dichloroethane | 258.4325 | 4.38 | 0.01 | 413408 | 65.0 | 31.4 | 2.1 | 62.1 |
| | | | | | 83.0 | 13.2 | 0.0 | 43.7 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 2,2-Dichloropropane | 253.0397 | 5.19 | -0.01 | 303307 | 41.0 | 67.7 | 36.5 | 96.5 |
| | | | | | 97.0 | 22.8 | 0.0 | 53.2 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,2-Dichloroethene | 261.8706 | 5.21 | 0.00 | 228170 | 61.0 | 161.6 | 137.2 | 197.2 |
| | | | | | 98.0 | 65.6 | 37.3 | 97.3 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|-----------|------|----------|--------|------|--------|-------|-------|
| Methyl ethyl ketone | 2688.2474 | 5.28 | 0.00 | 317271 | 72.0 | 20.8 | 0.0 | 51.3 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|-------|------|--------|-------|-------|
| Bromochloromethane | 247.0586 | 5.52 | 0.00 | 89178 | 49.0 | 190.0 | 152.9 | 212.9 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|------|--------|-------|-------|
| Chloroform | 248.0804 | 5.65 | 0.00 | 394946 | 85.0 | 64.9 | 36.0 | 96.0 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1,1-Trichloroethane | 258.7228 | 5.83 | 0.00 | 386005 | 99.0 | 64.4 | 34.7 | 94.7 |
| | | | | | 61.0 | 48.7 | 18.1 | 78.1 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Dibromofluoromethane | 259.0223 | 5.85 | 0.00 | 204073 | 191.5 | 22.5 | 0.0 | 53.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Carbon tetrachloride | 260.8774 | 6.03 | 0.00 | 383485 | 119.0 | 97.0 | 67.2 | 127.2 |
| | | | | | 121.0 | 30.9 | 0.1 | 60.1 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|-------|--------|-------|-------|
| 1,1-Dichloropropene | 264.6638 | 6.04 | 0.00 | 335741 | 110.0 | 35.6 | 5.9 | 65.9 |
| | | | | | 77.0 | 30.7 | 0.1 | 60.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 258.2324 | 6.24 | 0.00 | 87876 | 65.0 | 193.6 | 166.5 | 226.5 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|------|----------|--------|------|--------|-------|-------|
| Benzene | 257.5416 | 6.28 | 0.00 | 857534 | 77.0 | 23.6 | 0.0 | 53.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloroethane | 251.9675 | 6.32 | 0.00 | 226964 | 64.0 | 30.6 | 0.0 | 59.9 |
| | | | | | 98.0 | 7.4 | 0.0 | 37.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|----------|------|----------|--------|-------|--------|-------|-------|
| Trichloroethene | 262.2931 | 7.03 | 0.00 | 250285 | 130.0 | 101.7 | 71.5 | 131.5 |
| | | | | | 97.0 | 64.5 | 34.1 | 94.1 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloropropane | 254.7161 | 7.27 | 0.00 | 213800 | 76.0 | 38.5 | 8.2 | 68.2 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------|----------|------|----------|-------|-------|--------|-------|-------|
| Dibromomethane | 252.2734 | 7.40 | 0.00 | 89483 | 173.5 | 108.9 | 83.7 | 143.7 |
| | | | | | 95.0 | 83.1 | 52.2 | 112.2 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Bromodichloromethane | 257.2286 | 7.58 | 0.00 | 251805 | 85.0 | 64.3 | 34.5 | 94.5 |
| | | | | | 127.0 | 9.3 | 0.0 | 39.6 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,3-Dichloropropene | 265.2863 | 8.06 | 0.00 | 293617 | 39.0 | 53.0 | 23.3 | 83.3 |
| | | | | | 77.0 | 31.6 | 1.0 | 61.0 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 270.0265 | 8.32 | 0.00 | 823306 | 100.0 | 63.9 | 34.4 | 94.4 |
| | | | | | 99.0 | 9.4 | 0.0 | 39.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|------|----------|--------|------|--------|-------|-------|
| Toluene | 263.1330 | 8.39 | 0.00 | 541945 | 91.0 | 175.7 | 145.8 | 205.8 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|----------|------|----------|--------|------|--------|-------|-------|
| trans-1,3-Dichloropropene | 263.8027 | 8.64 | 0.00 | 207833 | 39.0 | 53.9 | 23.4 | 83.4 |
| | | | | | 77.0 | 35.1 | 2.4 | 62.4 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1,2-Trichloroethane | 248.2882 | 8.82 | 0.00 | 101888 | 97.0 | 114.4 | 84.6 | 144.6 |
| | | | | | 85.0 | 65.7 | 37.6 | 97.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Tetrachloroethene | 259.7419 | 8.94 | 0.00 | 218245 | 165.8 | 126.5 | 98.6 | 158.6 |
| | | | | | 129.0 | 90.3 | 61.5 | 121.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,3-Dichloropropane | 263.4754 | 8.98 | 0.00 | 212669 | 78.0 | 31.9 | 2.9 | 62.9 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Chlorodibromomethane | 258.3535 | 9.20 | 0.00 | 165695 | 127.0 | 77.8 | 48.0 | 108.0 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------|----------|------|----------|--------|-------|--------|-------|-------|
| 1,2-Dibromoethane | 257.8887 | 9.31 | 0.00 | 115714 | 109.0 | 94.6 | 64.5 | 124.5 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------|----------|------|----------|--------|-------|--------|-------|-------|
| Chlorobenzene | 258.2544 | 9.80 | 0.00 | 582326 | 114.0 | 32.1 | 2.1 | 62.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|----------|------|----------|--------|-------|--------|-------|-------|
| 1,1,1,2-Tetrachloroethane | 254.8274 | 9.89 | 0.00 | 200859 | 133.0 | 98.2 | 68.6 | 128.6 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|----------|------|----------|---------|-------|--------|-------|-------|
| Ethylbenzene | 266.8193 | 9.92 | 0.00 | 1043443 | 106.0 | 31.2 | 1.1 | 61.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------|----------|-------|----------|--------|------|--------|-------|-------|
| m+p-Xylenes | 543.4262 | 10.04 | 0.00 | 825866 | 91.0 | 201.4 | 171.4 | 231.4 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|-------|----------|--------|------|--------|-------|-------|
| o-Xylene | 270.4636 | 10.43 | 0.00 | 365914 | 91.0 | 213.0 | 183.1 | 243.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|-------|----------|--------|------|--------|-------|-------|
| Styrene | 278.0455 | 10.45 | 0.00 | 605646 | 78.0 | 50.3 | 19.6 | 79.6 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------|----------|-------|----------|-------|-------|--------|-------|-------|
| Bromoform | 257.5099 | 10.63 | 0.00 | 87836 | 170.5 | 51.9 | 22.1 | 82.1 |
| | | | | | 174.5 | 50.3 | 20.1 | 80.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 267.3186 | 10.95 | 0.00 | 261042 | 174.0 | 93.1 | 61.7 | 121.7 |
| | | | | | 176.0 | 89.6 | 60.6 | 120.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|----------|-------|----------|--------|-------|--------|-------|-------|
| Bromobenzene | 263.2944 | 11.09 | 0.00 | 227127 | 77.0 | 143.1 | 115.7 | 175.7 |
| | | | | | 158.0 | 96.5 | 66.5 | 126.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|----------|-------|----------|--------|------|--------|-------|-------|
| 1,1,2,2-Tetrachloroethane | 250.1577 | 11.11 | 0.00 | 124205 | 85.0 | 64.1 | 36.2 | 96.2 |












| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|----------|-------|----------|-------|-------|--------|-------|-------|
| 1,2,3-Trichloropropane | 249.2635 | 11.15 | 0.01 | 33115 | 112.0 | 65.5 | 33.5 | 93.5 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|----------|-------|----------|--------|------|--------|-------|-------|
| 2-Chlorotoluene | 267.2616 | 11.29 | 0.00 | 229396 | 91.0 | 283.3 | 252.3 | 312.3 |






Quantitation Results Report (QT Reviewed)
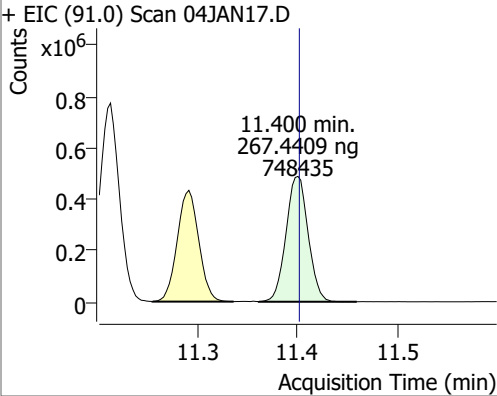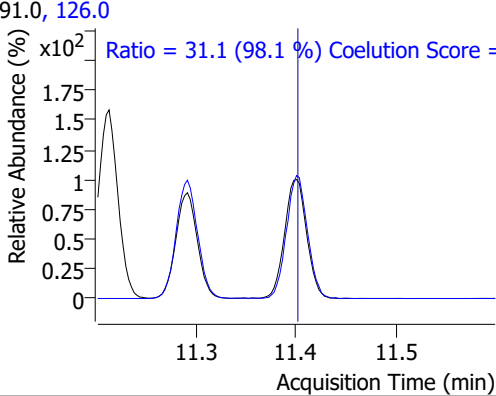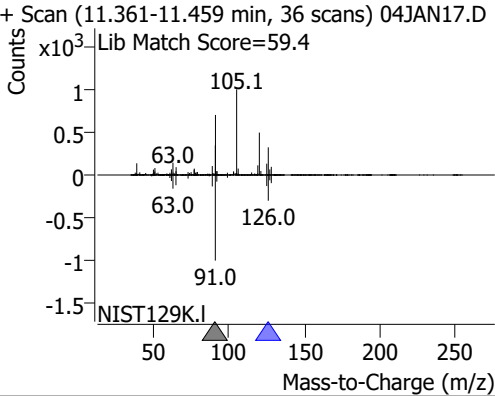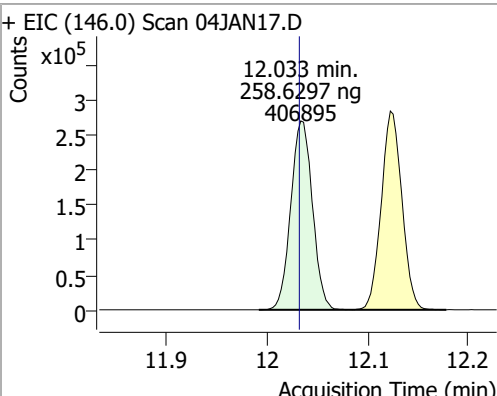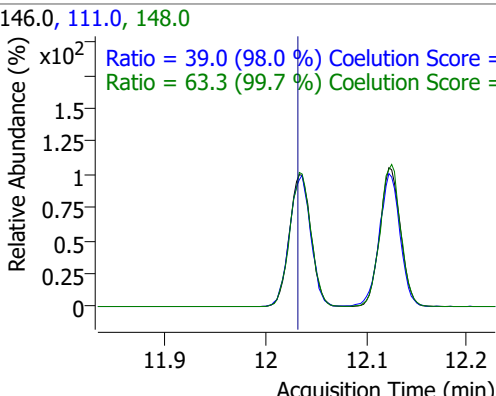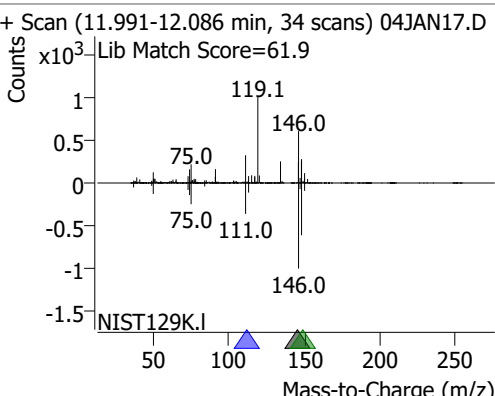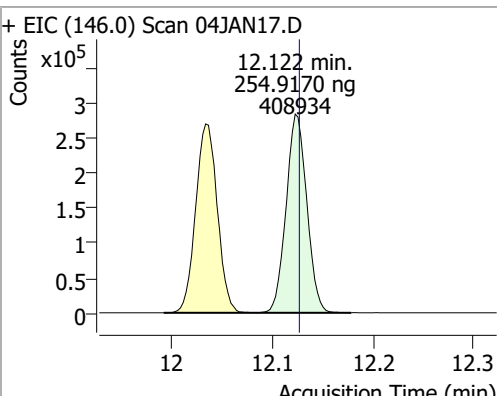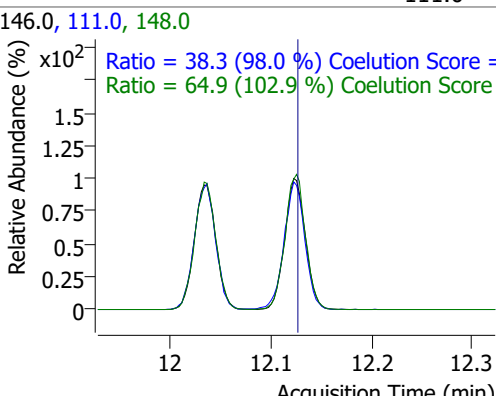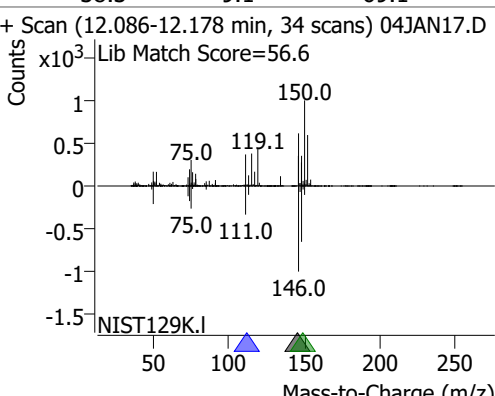
| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--|----------|-------|--|--------|-------|---|-------|-------|
| 4-Chlorotoluene | 267.4409 | 11.40 | 0.00 | 748435 | 126.0 | 31.1 | 1.7 | 61.7 |
| + EIC (91.0) Scan 04JAN17.D | | | 91.0, 126.0 | | | + Scan (11.361-11.459 min, 36 scans) 04JAN17.D | | |
|  | | |  | | |  | | |
| 1,3-Dichlorobenzene | 258.6297 | 12.03 | 0.00 | 406895 | 148.0 | 63.3 | 33.6 | 93.6 |
| + EIC (146.0) Scan 04JAN17.D | | | 146.0, 111.0, 148.0 | | | + Scan (11.991-12.086 min, 34 scans) 04JAN17.D | | |
|  | | |  | | |  | | |
| 1,4-Dichlorobenzene | 254.9170 | 12.12 | 0.00 | 408934 | 148.0 | 64.9 | 33.1 | 93.1 |
| + EIC (146.0) Scan 04JAN17.D | | | 146.0, 111.0, 148.0 | | | + Scan (12.086-12.178 min, 34 scans) 04JAN17.D | | |
|  | | |  | | |  | | |


Quantitation Results Report (QT Reviewed)

| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,2-Dichlorobenzene | 257.6524 | 12.49 | 0.00 | 342576 | 148.0 | 63.4 | 33.9 | 93.9 |
| | | | | | 111.0 | 40.5 | 11.0 | 71.0 |



Quantitation Results Report (QT Reviewed)

| | | | |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File | 04JAN19.D | Operator | MSC |
| Acq. Method | 5975CACQF.M | Acq. Date-Time | 1/4/2022 7:39:45 PM |
| Sample Name | ICAL010422_7 | Instrument | VOA5975C |
| Vial | 19 | Multiplier | 1.00 |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m | Comment | |
| Tune File | BFB_Atune3.u | Tune Date | 10/11/2021 4:02:00 PM |
| Batch Name | VG010422_8260B.batch.bin | Last Calib Update | 1/9/2022 8:59:52 PM |
| Ref Library | \\MASSHUNTER\Org\Library\NIST129K.I | | |



| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|----------|----|------|-------|-------|-------|----------|
|----------|----|------|-------|-------|-------|----------|

Internal Standards

| | | | | | | |
|--------------------------|--------|-------|--------|----------|----|--------|
| M Fluorobenzene | 6.621 | 96.0 | 841876 | 250.0000 | ng | -0.003 |
| M Chlorobenzene-d5 | 9.772 | 82.0 | 314668 | 250.0000 | ng | 0.000 |
| M 1,4-Dichlorobenzene-d4 | 12.100 | 152.0 | 266611 | 250.0000 | ng | 0.000 |

System Monitoring Compounds

| | | | | | | |
|-------------------------|----------------------|-------|---------|--------------------|----|--------|
| S Dibromofluoromethane | 5.848 | 113.0 | 305158 | 384.7503 | ng | 0.003 |
| Spiked Amount: 250.000 | Range: 80.0 - 119.0% | | | Recovery = 153.90% | * | |
| S 1,2-Dichloroethane-d4 | 6.233 | 67.0 | 129608 | 378.3335 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 81.0 - 118.0% | | | Recovery = 151.33% | * | |
| S Toluene-d8 | 8.322 | 98.0 | 1229775 | 405.5583 | ng | 0.003 |
| Spiked Amount: 250.000 | Range: 89.0 - 112.0% | | | Recovery = 162.22% | * | |
| S p-Bromofluorobenzene | 10.951 | 95.0 | 385474 | 394.6566 | ng | -0.003 |
| Spiked Amount: 250.000 | Range: 85.0 - 114.0% | | | Recovery = 157.86% | * | |

Target Compounds

| Compound | RT | QIon | Resp. | Conc. | Units | QValue |
|----------------------------------|-------|-------|--------|-----------|-------|--------|
| T Dichlorodifluoromethane | 1.241 | 85.0 | 412544 | 373.9449 | ng | 100 |
| T Chloromethane | 1.409 | 50.0 | 471454 | 352.0836 | ng | 99 |
| T Vinyl chloride | 1.498 | 62.0 | 448643 | 372.3564 | ng | 95 |
| T Bromomethane | 1.796 | 96.0 | 207491 | 385.1259 | ng | 98 |
| T Chloroethane | 1.897 | 64.0 | 217393 | 364.4573 | ng | 99 |
| T Trichlorofluoromethane | 2.145 | 101.0 | 555477 | 371.4290 | ng | 98 |
| T 1,1-Dichloroethene | 2.700 | 96.0 | 322557 | 380.3725 | ng | 100 |
| T Methylene chloride | 3.330 | 49.0 | 435116 | 348.0666 | ng | 99 |
| T trans-1,2-Dichloroethene | 3.715 | 96.0 | 325415 | 376.1367 | ng | 97 |
| T Methyl tert-butyl ether (MTBE) | 3.751 | 73.0 | 437439 | 391.1767 | ng | 100 |
| T 1,1-Dichloroethane | 4.381 | 63.0 | 612660 | 380.4437 | ng | 99 |
| T 2,2-Dichloropropane | 5.190 | 77.0 | 446282 | 369.8436 | ng | 100 |
| T cis-1,2-Dichloroethene | 5.212 | 96.0 | 339211 | 386.7236 | ng | 97 |
| T Methyl ethyl ketone | 5.279 | 43.0 | 470653 | 3961.3410 | ng | 100 |
| T Bromochloromethane | 5.516 | 128.0 | 135103 | 371.8004 | ng | 99 |
| T Chloroform | 5.650 | 83.0 | 588080 | 366.9389 | ng | 99 |

Quantitation Results Report (QT Reviewed)

| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|-----------------------------|--------|-------|---------|----------|-------|----------|
| T 1,1,1-Trichloroethane | 5.831 | 97.0 | 580748 | 386.6625 | ng | 99 |
| T Carbon tetrachloride | 6.024 | 117.0 | 572545 | 386.9014 | ng | 99 |
| T 1,1-Dichloropropene | 6.040 | 75.0 | 507157 | 397.1322 | ng | 100 |
| T Benzene | 6.278 | 78.0 | 1293370 | 385.8526 | ng | 99 |
| T 1,2-Dichloroethane | 6.322 | 62.0 | 332775 | 366.9787 | ng | 97 |
| T Trichloroethene | 7.028 | 95.0 | 374370 | 394.4896 | ng | 99 |
| T 1,2-Dichloropropane | 7.270 | 63.0 | 324602 | 388.8502 | ng | 98 |
| T Dibromomethane | 7.396 | 93.0 | 134282 | 380.6547 | ng | 96 |
| T Bromodichloromethane | 7.585 | 83.0 | 375983 | 386.1940 | ng | 100 |
| T cis-1,3-Dichloropropene | 8.057 | 75.0 | 441168 | 400.7930 | ng | 99 |
| T Toluene | 8.388 | 92.0 | 813204 | 397.0106 | ng | 100 |
| T trans-1,3-Dichloropropene | 8.639 | 75.0 | 315063 | 402.1098 | ng | 99 |
| T 1,1,2-Trichloroethane | 8.818 | 83.0 | 152331 | 373.2534 | ng | 100 |
| T Tetrachloroethene | 8.938 | 163.8 | 319950 | 382.8796 | ng | 99 |
| T 1,3-Dichloropropane | 8.980 | 76.0 | 312547 | 389.3442 | ng | 99 |
| T Chlorodibromomethane | 9.203 | 129.0 | 247279 | 387.6812 | ng | 99 |
| T 1,2-Dibromoethane | 9.306 | 107.0 | 168577 | 377.7698 | ng | 100 |
| T Chlorobenzene | 9.802 | 112.0 | 867732 | 386.9455 | ng | 100 |
| T 1,1,1,2-Tetrachloroethane | 9.892 | 131.0 | 307436 | 392.1859 | ng | 96 |
| T Ethylbenzene | 9.919 | 91.0 | 1574219 | 404.7587 | ng | 100 |
| T m+p-Xylenes | 10.039 | 106.0 | 1228570 | 812.8556 | ng | 100 |
| T o-Xylene | 10.433 | 106.0 | 549244 | 408.2043 | ng | 100 |
| T Styrene | 10.447 | 104.0 | 896331 | 413.7595 | ng | 99 |
| T Bromoform | 10.628 | 172.5 | 129038 | 378.2200 | ng | 99 |
| T Bromobenzene | 11.093 | 156.0 | 333431 | 386.4420 | ng | 98 |
| T 1,1,2,2-Tetrachloroethane | 11.110 | 83.0 | 182470 | 367.4276 | ng | 98 |
| T 1,2,3-Trichloropropane | 11.149 | 110.0 | 48325 | 363.6732 | ng | 100 |
| T 2-Chlorotoluene | 11.291 | 126.0 | 336386 | 391.8269 | ng | 98 |
| T 4-Chlorotoluene | 11.400 | 91.0 | 1109221 | 396.2756 | ng | 100 |
| T 1,3-Dichlorobenzene | 12.033 | 146.0 | 603674 | 383.6225 | ng | 100 |
| T 1,4-Dichlorobenzene | 12.125 | 146.0 | 595919 | 371.3969 | ng | 98 |
| T 1,2-Dichlorobenzene | 12.493 | 146.0 | 499147 | 375.3283 | ng | 99 |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------------|----------|------|----------------|--------|------|--|-------|-------|
| Dichlorodifluoromethane | 373.9449 | 1.24 | 0.00 | 412544 | 87.0 | 32.5 | 2.3 | 62.3 |
| + EIC (85.0) Scan 04JAN19.D | | | 85.0, 87.0 | | | + Scan (1.213-1.406 min, 70 scans) 04JAN19.D Lib Match Score=80.8 | | |
| | | | | | | Ratio = 32.5 (100.7 %) Coelution Score | | |
| Chloromethane | 352.0836 | 1.41 | 0.00 | 471454 | 52.0 | 32.6 | 2.1 | 62.1 |
| + EIC (50.0) Scan 04JAN19.D | | | 50.0, 52.0 | | | + Scan (1.375-1.484 min, 40 scans) 04JAN19.D Lib Match Score=87.6 | | |
| | | | | | | Ratio = 32.6 (101.3 %) Coelution Score | | |
| Vinyl chloride | 372.3564 | 1.50 | 0.00 | 448643 | 64.0 | 32.8 | 0.0 | 59.9 |
| + EIC (62.0) Scan 04JAN19.D | | | 62.0, 64.0 | | | + Scan (1.462-1.657 min, 70 scans) 04JAN19.D Lib Match Score=87.2 | | |
| | | | | | | Ratio = 32.8 (109.8 %) Coelution Score | | |
| Bromomethane | 385.1259 | 1.80 | 0.00 | 207491 | 94.0 | 106.2 | 74.6 | 134.6 |
| + EIC (96.0) Scan 04JAN19.D | | | 96.0, 94.0 | | | + Scan (1.760-1.919 min, 58 scans) 04JAN19.D Lib Match Score=74.9 | | |
| | | | | | | Ratio = 106.2 (101.5 %) Coelution Score | | |

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|----------|------|----------|--------|------|--------|-------|-------|
| Chloroethane | 364.4573 | 1.90 | 0.00 | 217393 | 66.0 | 30.9 | 0.1 | 60.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Trichlorofluoromethane | 371.4290 | 2.14 | 0.00 | 555477 | 103.0 | 65.6 | 34.2 | 94.2 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1-Dichloroethene | 380.3725 | 2.70 | 0.00 | 322557 | 61.0 | 180.6 | 150.3 | 210.3 |
| | | | | | 63.0 | 57.2 | 26.7 | 86.7 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| Methylene chloride | 348.0666 | 3.33 | -0.01 | 435116 | 84.0 | 66.5 | 36.9 | 96.9 |
| | | | | | 86.0 | 42.7 | 14.3 | 74.3 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------------|----------|------|----------|--------|------|--------|-------|-------|
| trans-1,2-Dichloroethene | 376.1367 | 3.71 | 0.00 | 325415 | 61.0 | 158.9 | 123.9 | 183.9 |
| | | | | | 98.0 | 63.7 | 35.7 | 95.7 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------------------|----------|------|----------|--------|------|--------|-------|-------|
| Methyl tert-butyl ether (MTBE) | 391.1767 | 3.75 | 0.00 | 437439 | 57.0 | 24.4 | 0.0 | 54.6 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1-Dichloroethane | 380.4437 | 4.38 | 0.00 | 612660 | 65.0 | 31.4 | 2.1 | 62.1 |
| | | | | | 83.0 | 13.1 | 0.0 | 43.7 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 2,2-Dichloropropane | 369.8436 | 5.19 | -0.01 | 446282 | 41.0 | 66.5 | 36.5 | 96.5 |
| | | | | | 97.0 | 23.5 | 0.0 | 53.2 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,2-Dichloroethene | 386.7236 | 5.21 | 0.00 | 339211 | 61.0 | 162.9 | 137.2 | 197.2 |
| | | | | | 98.0 | 64.4 | 37.3 | 97.3 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|-----------|------|----------|--------|------|--------|-------|-------|
| Methyl ethyl ketone | 3961.3410 | 5.28 | 0.00 | 470653 | 72.0 | 21.5 | 0.0 | 51.3 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| Bromochloromethane | 371.8004 | 5.52 | 0.00 | 135103 | 49.0 | 184.8 | 152.9 | 212.9 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|------|--------|-------|-------|
| Chloroform | 366.9389 | 5.65 | 0.00 | 588080 | 85.0 | 65.5 | 36.0 | 96.0 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1,1-Trichloroethane | 386.6625 | 5.83 | 0.00 | 580748 | 99.0 | 64.2 | 34.7 | 94.7 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Dibromofluoromethane | 384.7503 | 5.85 | 0.00 | 305158 | 191.5 | 22.0 | 0.0 | 53.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Carbon tetrachloride | 386.9014 | 6.02 | 0.00 | 572545 | 119.0 | 96.4 | 67.2 | 127.2 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|-------|--------|-------|-------|
| 1,1-Dichloropropene | 397.1322 | 6.04 | 0.00 | 507157 | 110.0 | 36.0 | 5.9 | 65.9 |
| | | | | | 77.0 | 30.5 | 0.1 | 60.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 378.3335 | 6.23 | 0.00 | 129608 | 65.0 | 196.4 | 166.5 | 226.5 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|------|----------|---------|------|--------|-------|-------|
| Benzene | 385.8526 | 6.28 | 0.00 | 1293370 | 77.0 | 23.3 | 0.0 | 53.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloroethane | 366.9787 | 6.32 | 0.00 | 332775 | 64.0 | 31.9 | 0.0 | 59.9 |
| | | | | | 98.0 | 7.9 | 0.0 | 37.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|----------|------|----------|--------|-------|--------|-------|-------|
| Trichloroethene | 394.4896 | 7.03 | 0.00 | 374370 | 130.0 | 102.7 | 71.5 | 131.5 |
| | | | | | 97.0 | 64.4 | 34.1 | 94.1 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloropropane | 388.8502 | 7.27 | 0.00 | 324602 | 76.0 | 39.1 | 8.2 | 68.2 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------|----------|------|----------|--------|-------|--------|-------|-------|
| Dibromomethane | 380.6547 | 7.40 | 0.00 | 134282 | 173.5 | 107.8 | 83.7 | 143.7 |
| | | | | | 95.0 | 83.6 | 52.2 | 112.2 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Bromodichloromethane | 386.1940 | 7.59 | 0.00 | 375983 | 85.0 | 64.5 | 34.5 | 94.5 |
| | | | | | 127.0 | 9.2 | 0.0 | 39.6 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,3-Dichloropropene | 400.7930 | 8.06 | 0.00 | 441168 | 39.0 | 52.9 | 23.3 | 83.3 |
| | | | | | 77.0 | 31.8 | 1.0 | 61.0 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|---------|-------|--------|-------|-------|
| Toluene-d8 | 405.5583 | 8.32 | 0.00 | 1229775 | 100.0 | 64.2 | 34.4 | 94.4 |
| | | | | | 99.0 | 9.4 | 0.0 | 39.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|------|----------|--------|------|--------|-------|-------|
| Toluene | 397.0106 | 8.39 | 0.00 | 813204 | 91.0 | 175.4 | 145.8 | 205.8 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|----------|------|----------|--------|------|--------|-------|-------|
| trans-1,3-Dichloropropene | 402.1098 | 8.64 | 0.00 | 315063 | 39.0 | 52.3 | 23.4 | 83.4 |
| | | | | | 77.0 | 32.6 | 2.4 | 62.4 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1,2-Trichloroethane | 373.2534 | 8.82 | 0.00 | 152331 | 97.0 | 114.6 | 84.6 | 144.6 |
| | | | | | 85.0 | 66.7 | 37.6 | 97.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Tetrachloroethene | 382.8796 | 8.94 | 0.00 | 319950 | 165.8 | 130.7 | 98.6 | 158.6 |
| | | | | | 129.0 | 91.3 | 61.5 | 121.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,3-Dichloropropane | 389.3442 | 8.98 | 0.00 | 312547 | 78.0 | 32.2 | 2.9 | 62.9 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Chlorodibromomethane | 387.6812 | 9.20 | 0.00 | 247279 | 127.0 | 77.1 | 48.0 | 108.0 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------|----------|------|----------|--------|-------|--------|-------|-------|
| 1,2-Dibromoethane | 377.7698 | 9.31 | 0.00 | 168577 | 109.0 | 94.6 | 64.5 | 124.5 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------|----------|------|----------|--------|-------|--------|-------|-------|
| Chlorobenzene | 386.9455 | 9.80 | 0.00 | 867732 | 114.0 | 32.3 | 2.1 | 62.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|----------|------|----------|--------|-------|--------|-------|-------|
| 1,1,1,2-Tetrachloroethane | 392.1859 | 9.89 | 0.00 | 307436 | 133.0 | 94.2 | 68.6 | 128.6 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|----------|------|----------|---------|-------|--------|-------|-------|
| Ethylbenzene | 404.7587 | 9.92 | 0.00 | 1574219 | 106.0 | 31.1 | 1.1 | 61.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------|----------|-------|----------|---------|------|--------|-------|-------|
| m+p-Xylenes | 812.8556 | 10.04 | 0.00 | 1228570 | 91.0 | 201.2 | 171.4 | 231.4 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|-------|----------|--------|------|--------|-------|-------|
| o-Xylene | 408.2043 | 10.43 | 0.00 | 549244 | 91.0 | 213.2 | 183.1 | 243.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|-------|----------|--------|------|--------|-------|-------|
| Styrene | 413.7595 | 10.45 | 0.00 | 896331 | 78.0 | 50.0 | 19.6 | 79.6 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------|----------|-------|----------|--------|-------|--------|-------|-------|
| Bromoform | 378.2200 | 10.63 | 0.00 | 129038 | 170.5 | 52.5 | 22.1 | 82.1 |
| | | | | | 174.5 | 50.4 | 20.1 | 80.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 394.6566 | 10.95 | 0.00 | 385474 | 174.0 | 94.4 | 61.7 | 121.7 |
| | | | | | 176.0 | 92.3 | 60.6 | 120.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|----------|-------|----------|--------|-------|--------|-------|-------|
| Bromobenzene | 386.4420 | 11.09 | 0.00 | 333431 | 77.0 | 142.7 | 115.7 | 175.7 |
| | | | | | 158.0 | 98.4 | 66.5 | 126.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|----------|-------|----------|--------|------|--------|-------|-------|
| 1,1,2,2-Tetrachloroethane | 367.4276 | 11.11 | -0.01 | 182470 | 85.0 | 64.9 | 36.2 | 96.2 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|----------|-------|----------|-------|-------|--------|-------|-------|
| 1,2,3-Trichloropropane | 363.6732 | 11.15 | 0.00 | 48325 | 112.0 | 63.7 | 33.5 | 93.5 |






| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|----------|-------|----------|--------|------|--------|-------|-------|
| 2-Chlorotoluene | 391.8269 | 11.29 | 0.00 | 336386 | 91.0 | 285.3 | 252.3 | 312.3 |






Quantitation Results Report (QT Reviewed)




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|----------|-------|----------|---------|-------|--------|-------|-------|
| 4-Chlorotoluene | 396.2756 | 11.40 | 0.00 | 1109221 | 126.0 | 31.5 | 1.7 | 61.7 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,3-Dichlorobenzene | 383.6225 | 12.03 | 0.00 | 603674 | 148.0 | 63.5 | 33.6 | 93.6 |
| | | | | | 111.0 | 39.3 | 9.8 | 69.8 |






| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,4-Dichlorobenzene | 371.3969 | 12.13 | 0.00 | 595919 | 148.0 | 64.9 | 33.1 | 93.1 |
| | | | | | 111.0 | 38.5 | 9.1 | 69.1 |




Quantitation Results Report (QT Reviewed)

| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,2-Dichlorobenzene | 375.3283 | 12.49 | 0.00 | 499147 | 148.0 | 63.8 | 33.9 | 93.9 |
| | | | | | 111.0 | 40.2 | 11.0 | 71.0 |



Quantitation Results Report (QT Reviewed)

| | | | |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File | 04JAN21.D | Operator | MSC |
| Acq. Method | 5975CACQF.M | Acq. Date-Time | 1/4/2022 8:34:31 PM |
| Sample Name | ICAL010422_8 | Instrument | VOA5975C |
| Vial | 21 | Multiplier | 1.00 |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m | Comment | |
| Tune File | BFB_Atune3.u | Tune Date | 10/11/2021 4:02:00 PM |
| Batch Name | VG010422_8260B.batch.bin | Last Calib Update | 1/9/2022 8:59:52 PM |
| Ref Library | \\MASSHUNTER\Org\Library\NIST129K.I | | |















| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|------------------------------------|----------------------|-------|---------|--------------------|-------|----------|
| Internal Standards | | | | | | |
| M Fluorobenzene | 6.621 | 96.0 | 841364 | 250.0000 | ng | -0.003 |
| M Chlorobenzene-d5 | 9.774 | 82.0 | 313585 | 250.0000 | ng | 0.003 |
| M 1,4-Dichlorobenzene-d4 | 12.103 | 152.0 | 262971 | 250.0000 | ng | 0.003 |
| System Monitoring Compounds | | | | | | |
| S Dibromofluoromethane | 5.845 | 113.0 | 404568 | 510.3991 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 80.0 - 119.0% | | | Recovery = 204.16% | * | |
| S 1,2-Dichloroethane-d4 | 6.233 | 67.0 | 174713 | 510.3080 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 81.0 - 118.0% | | | Recovery = 204.12% | * | |
| S Toluene-d8 | 8.319 | 98.0 | 1644540 | 544.2136 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 89.0 - 112.0% | | | Recovery = 217.69% | * | |
| S p-Bromofluorobenzene | 10.949 | 95.0 | 521580 | 541.3964 | ng | -0.006 |
| Spiked Amount: 250.000 | Range: 85.0 - 114.0% | | | Recovery = 216.56% | * | |
| Target Compounds | | | | | | |
| T Dichlorodifluoromethane | 1.241 | 85.0 | 545484 | 494.7474 | ng | 99 |
| T Chloromethane | 1.406 | 50.0 | 642582 | 480.1747 | ng | 100 |
| T Vinyl chloride | 1.495 | 62.0 | 600092 | 498.3563 | ng | 95 |
| T Bromomethane | 1.793 | 96.0 | 277301 | 515.0141 | ng | 98 |
| T Chloroethane | 1.894 | 64.0 | 287041 | 481.5143 | ng | 98 |
| T Trichlorofluoromethane | 2.145 | 101.0 | 731829 | 489.6475 | ng | 99 |
| T 1,1-Dichloroethene | 2.700 | 96.0 | 436507 | 515.0603 | ng | 98 |
| T Methylene chloride | 3.330 | 49.0 | 583438 | 466.9993 | ng | 98 |
| T trans-1,2-Dichloroethene | 3.718 | 96.0 | 440967 | 510.0097 | ng | 98 |
| T Methyl tert-butyl ether (MTBE) | 3.754 | 73.0 | 584294 | 522.8187 | ng | 99 |
| T 1,1-Dichloroethane | 4.378 | 63.0 | 829359 | 515.3207 | ng | 99 |
| T 2,2-Dichloropropane | 5.190 | 77.0 | 601823 | 499.0473 | ng | 98 |
| T cis-1,2-Dichloroethene | 5.212 | 96.0 | 452377 | 516.0544 | ng | 99 |
| T Methyl ethyl ketone | 5.279 | 43.0 | 632539 | 5327.1253 | ng | 99 |
| T Bromochloromethane | 5.519 | 128.0 | 179618 | 494.6054 | ng | 98 |
| T Chloroform | 5.653 | 83.0 | 783422 | 489.1221 | ng | 99 |

Quantitation Results Report (QT Reviewed)

| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|-----------------------------|--------|-------|---------|-----------|-------|----------|
| T 1,1,1-Trichloroethane | 5.834 | 97.0 | 778785 | 518.8312 | ng | 99 |
| T Carbon tetrachloride | 6.024 | 117.0 | 770907 | 521.2630 | ng | 98 |
| T 1,1-Dichloropropene | 6.038 | 75.0 | 693669 | 543.5121 | ng | 99 |
| T Benzene | 6.280 | 78.0 | 1714050 | 511.6658 | ng | 100 |
| T 1,2-Dichloroethane | 6.322 | 62.0 | 450739 | 497.3699 | ng | 100 |
| T Trichloroethene | 7.028 | 95.0 | 505400 | 534.4007 | ng | 99 |
| T 1,2-Dichloropropane | 7.270 | 63.0 | 436057 | 524.1695 | ng | 100 |
| T Dibromomethane | 7.396 | 93.0 | 176038 | 500.7456 | ng | 98 |
| T Bromodichloromethane | 7.585 | 83.0 | 502929 | 518.3718 | ng | 100 |
| T cis-1,3-Dichloropropene | 8.059 | 75.0 | 591147 | 538.9008 | ng | 99 |
| T Toluene | 8.389 | 92.0 | 1095161 | 536.5101 | ng | 99 |
| T trans-1,3-Dichloropropene | 8.637 | 75.0 | 416771 | 533.7551 | ng | 99 |
| T 1,1,2-Trichloroethane | 8.815 | 83.0 | 205463 | 505.1803 | ng | 97 |
| T Tetrachloroethene | 8.938 | 163.8 | 428812 | 514.9255 | ng | 100 |
| T 1,3-Dichloropropane | 8.980 | 76.0 | 408993 | 511.2479 | ng | 100 |
| T Chlorodibromomethane | 9.203 | 129.0 | 330813 | 520.4361 | ng | 99 |
| T 1,2-Dibromoethane | 9.303 | 107.0 | 225877 | 507.9234 | ng | 99 |
| T Chlorobenzene | 9.802 | 112.0 | 1153147 | 515.9957 | ng | 100 |
| T 1,1,1,2-Tetrachloroethane | 9.892 | 131.0 | 406450 | 520.2855 | ng | 98 |
| T Ethylbenzene | 9.919 | 91.0 | 2111152 | 544.6881 | ng | 100 |
| T m+p-Xylenes | 10.039 | 106.0 | 1637879 | 1087.4082 | ng | 99 |
| T o-Xylene | 10.430 | 106.0 | 734101 | 547.4764 | ng | 100 |
| T Styrene | 10.449 | 104.0 | 1199879 | 555.7946 | ng | 99 |
| T Bromoform | 10.625 | 172.5 | 175918 | 522.7660 | ng | 98 |
| T Bromobenzene | 11.094 | 156.0 | 439147 | 516.0104 | ng | 98 |
| T 1,1,2,2-Tetrachloroethane | 11.113 | 83.0 | 240837 | 491.6700 | ng | 99 |
| T 1,2,3-Trichloropropane | 11.146 | 110.0 | 64422 | 491.5229 | ng | 99 |
| T 2-Chlorotoluene | 11.292 | 126.0 | 455991 | 538.4964 | ng | 99 |
| T 4-Chlorotoluene | 11.400 | 91.0 | 1468376 | 531.8471 | ng | 100 |
| T 1,3-Dichlorobenzene | 12.033 | 146.0 | 793993 | 511.5504 | ng | 100 |
| T 1,4-Dichlorobenzene | 12.125 | 146.0 | 794954 | 502.3001 | ng | 99 |
| T 1,2-Dichlorobenzene | 12.493 | 146.0 | 664247 | 506.3871 | ng | 99 |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)

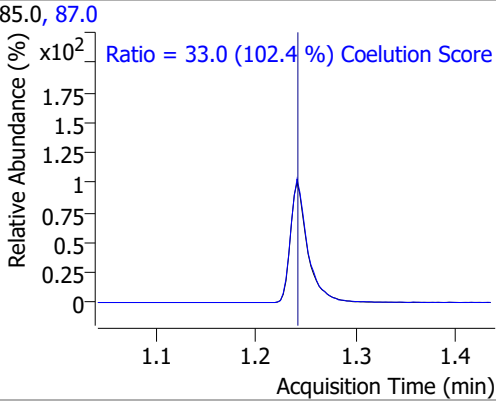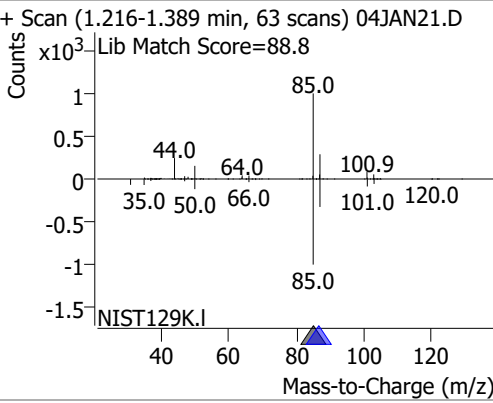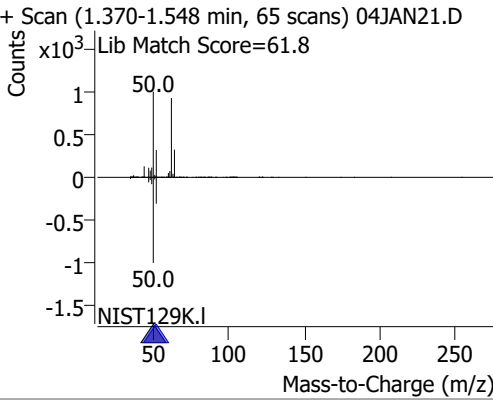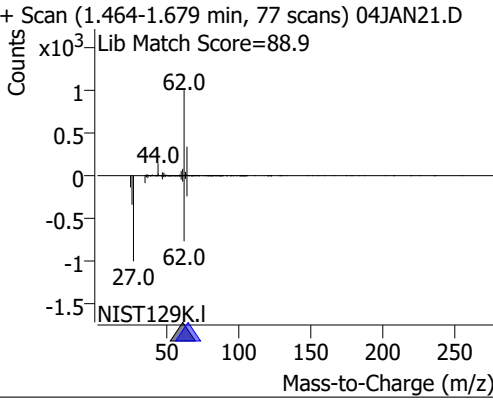
| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---|----------|------|--|--------|------|---|-------|-------|
| Dichlorodifluoromethane | 494.7474 | 1.24 | 0.00 | 545484 | 87.0 | 33.0 | 2.3 | 62.3 |
| + EIC (85.0) Scan 04JAN21.D  | | | 85.0, 87.0  | | | + Scan (1.216-1.389 min, 63 scans) 04JAN21.D Lib Match Score=88.8  | | |
| Chloromethane | 480.1747 | 1.41 | 0.00 | 642582 | 52.0 | 32.1 | 2.1 | 62.1 |
| + EIC (50.0) Scan 04JAN21.D  | | | 50.0, 52.0  | | | + Scan (1.370-1.548 min, 65 scans) 04JAN21.D Lib Match Score=61.8  | | |
| Vinyl chloride | 498.3563 | 1.50 | 0.00 | 600092 | 64.0 | 32.5 | 0.0 | 59.9 |
| + EIC (62.0) Scan 04JAN21.D  | | | 62.0, 64.0  | | | + Scan (1.464-1.679 min, 77 scans) 04JAN21.D Lib Match Score=88.9  | | |
| Bromomethane | 515.0141 | 1.79 | -0.01 | 277301 | 94.0 | 106.8 | 74.6 | 134.6 |
| + EIC (96.0) Scan 04JAN21.D  | | | 96.0, 94.0  | | | + Scan (1.757-1.941 min, 67 scans) 04JAN21.D Lib Match Score=74.7  | | |

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|----------|------|----------|--------|------|--------|-------|-------|
| Chloroethane | 481.5143 | 1.89 | 0.00 | 287041 | 66.0 | 31.4 | 0.1 | 60.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Trichlorofluoromethane | 489.6475 | 2.14 | 0.00 | 731829 | 103.0 | 64.7 | 34.2 | 94.2 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1-Dichloroethene | 515.0603 | 2.70 | 0.00 | 436507 | 61.0 | 184.2 | 150.3 | 210.3 |
| | | | | | 63.0 | 57.2 | 26.7 | 86.7 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| Methylene chloride | 466.9993 | 3.33 | -0.01 | 583438 | 84.0 | 66.3 | 36.9 | 96.9 |
| | | | | | 86.0 | 42.3 | 14.3 | 74.3 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------------|----------|------|----------|--------|------|--------|-------|-------|
| trans-1,2-Dichloroethene | 510.0097 | 3.72 | 0.00 | 440967 | 61.0 | 157.1 | 123.9 | 183.9 |
| | | | | | 98.0 | 64.1 | 35.7 | 95.7 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------------------|----------|------|----------|--------|------|--------|-------|-------|
| Methyl tert-butyl ether (MTBE) | 522.8187 | 3.75 | 0.00 | 584294 | 57.0 | 24.9 | 0.0 | 54.6 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1-Dichloroethane | 515.3207 | 4.38 | 0.00 | 829359 | 65.0 | 31.6 | 2.1 | 62.1 |
| | | | | | 83.0 | 12.8 | 0.0 | 43.7 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 2,2-Dichloropropane | 499.0473 | 5.19 | -0.01 | 601823 | 41.0 | 64.7 | 36.5 | 96.5 |
| | | | | | 97.0 | 22.9 | 0.0 | 53.2 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,2-Dichloroethene | 516.0544 | 5.21 | 0.00 | 452377 | 61.0 | 166.1 | 137.2 | 197.2 |
| | | | | | 98.0 | 65.6 | 37.3 | 97.3 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|-----------|------|----------|--------|------|--------|-------|-------|
| Methyl ethyl ketone | 5327.1253 | 5.28 | 0.00 | 632539 | 72.0 | 21.6 | 0.0 | 51.3 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| Bromochloromethane | 494.6054 | 5.52 | 0.00 | 179618 | 49.0 | 186.2 | 152.9 | 212.9 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|------|--------|-------|-------|
| Chloroform | 489.1221 | 5.65 | 0.00 | 783422 | 85.0 | 65.4 | 36.0 | 96.0 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1,1-Trichloroethane | 518.8312 | 5.83 | 0.00 | 778785 | 99.0 | 64.1 | 34.7 | 94.7 |
| | | | | | 61.0 | 48.2 | 18.1 | 78.1 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Dibromofluoromethane | 510.3991 | 5.85 | 0.00 | 404568 | 191.5 | 22.4 | 0.0 | 53.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Carbon tetrachloride | 521.2630 | 6.02 | 0.00 | 770907 | 119.0 | 95.3 | 67.2 | 127.2 |
| | | | | | 121.0 | 31.1 | 0.1 | 60.1 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|-------|--------|-------|-------|
| 1,1-Dichloropropene | 543.5121 | 6.04 | 0.00 | 693669 | 110.0 | 35.6 | 5.9 | 65.9 |
| | | | | | 77.0 | 30.8 | 0.1 | 60.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 510.3080 | 6.23 | 0.00 | 174713 | 65.0 | 194.7 | 166.5 | 226.5 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|------|----------|---------|------|--------|-------|-------|
| Benzene | 511.6658 | 6.28 | 0.00 | 1714050 | 77.0 | 23.5 | 0.0 | 53.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloroethane | 497.3699 | 6.32 | 0.00 | 450739 | 64.0 | 30.0 | 0.0 | 59.9 |
| | | | | | 98.0 | 7.4 | 0.0 | 37.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|----------|------|----------|--------|-------|--------|-------|-------|
| Trichloroethene | 534.4007 | 7.03 | 0.00 | 505400 | 130.0 | 103.0 | 71.5 | 131.5 |
| | | | | | 97.0 | 65.2 | 34.1 | 94.1 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloropropane | 524.1695 | 7.27 | 0.00 | 436057 | 76.0 | 38.1 | 8.2 | 68.2 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------|----------|------|----------|--------|-------|--------|-------|-------|
| Dibromomethane | 500.7456 | 7.40 | 0.00 | 176038 | 173.5 | 109.8 | 83.7 | 143.7 |
| | | | | | 95.0 | 82.8 | 52.2 | 112.2 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Bromodichloromethane | 518.3718 | 7.59 | 0.00 | 502929 | 85.0 | 64.7 | 34.5 | 94.5 |
| | | | | | 127.0 | 9.4 | 0.0 | 39.6 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,3-Dichloropropene | 538.9008 | 8.06 | 0.00 | 591147 | 39.0 | 52.4 | 23.3 | 83.3 |
| | | | | | 77.0 | 31.4 | 1.0 | 61.0 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|---------|-------|--------|-------|-------|
| Toluene-d8 | 544.2136 | 8.32 | 0.00 | 1644540 | 100.0 | 64.1 | 34.4 | 94.4 |
| | | | | | 99.0 | 9.5 | 0.0 | 39.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|------|----------|---------|------|--------|-------|-------|
| Toluene | 536.5101 | 8.39 | 0.00 | 1095161 | 91.0 | 174.1 | 145.8 | 205.8 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|----------|------|----------|--------|------|--------|-------|-------|
| trans-1,3-Dichloropropene | 533.7551 | 8.64 | 0.00 | 416771 | 39.0 | 52.3 | 23.4 | 83.4 |
| | | | | | 77.0 | 33.0 | 2.4 | 62.4 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1,2-Trichloroethane | 505.1803 | 8.82 | 0.00 | 205463 | 97.0 | 112.6 | 84.6 | 144.6 |
| | | | | | 85.0 | 63.1 | 37.6 | 97.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Tetrachloroethene | 514.9255 | 8.94 | 0.00 | 428812 | 165.8 | 129.5 | 98.6 | 158.6 |
| | | | | | 129.0 | 91.5 | 61.5 | 121.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,3-Dichloropropane | 511.2479 | 8.98 | 0.00 | 408993 | 78.0 | 32.9 | 2.9 | 62.9 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Chlorodibromomethane | 520.4361 | 9.20 | 0.00 | 330813 | 127.0 | 76.7 | 48.0 | 108.0 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------|----------|------|----------|--------|-------|--------|-------|-------|
| 1,2-Dibromoethane | 507.9234 | 9.30 | 0.00 | 225877 | 109.0 | 95.9 | 64.5 | 124.5 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------|----------|------|----------|---------|-------|--------|-------|-------|
| Chlorobenzene | 515.9957 | 9.80 | 0.00 | 1153147 | 114.0 | 32.0 | 2.1 | 62.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|----------|------|----------|--------|-------|--------|-------|-------|
| 1,1,1,2-Tetrachloroethane | 520.2855 | 9.89 | 0.00 | 406450 | 133.0 | 96.1 | 68.6 | 128.6 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|----------|------|----------|---------|-------|--------|-------|-------|
| Ethylbenzene | 544.6881 | 9.92 | 0.00 | 2111152 | 106.0 | 31.4 | 1.1 | 61.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------|-----------|-------|----------|---------|------|--------|-------|-------|
| m+p-Xylenes | 1087.4082 | 10.04 | 0.00 | 1637879 | 91.0 | 202.4 | 171.4 | 231.4 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|-------|----------|--------|------|--------|-------|-------|
| o-Xylene | 547.4764 | 10.43 | 0.00 | 734101 | 91.0 | 213.0 | 183.1 | 243.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|-------|----------|---------|------|--------|-------|-------|
| Styrene | 555.7946 | 10.45 | 0.00 | 1199879 | 78.0 | 50.2 | 19.6 | 79.6 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------|----------|-------|----------|--------|-------|--------|-------|-------|
| Bromoform | 522.7660 | 10.63 | 0.00 | 175918 | 170.5 | 51.3 | 22.1 | 82.1 |
| | | | | | 174.5 | 48.1 | 20.1 | 80.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 541.3964 | 10.95 | -0.01 | 521580 | 174.0 | 93.3 | 61.7 | 121.7 |
| | | | | | 176.0 | 89.7 | 60.6 | 120.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|----------|-------|----------|--------|-------|--------|-------|-------|
| Bromobenzene | 516.0104 | 11.09 | 0.00 | 439147 | 77.0 | 142.6 | 115.7 | 175.7 |
| | | | | | 158.0 | 97.9 | 66.5 | 126.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|----------|-------|----------|--------|------|--------|-------|-------|
| 1,1,2,2-Tetrachloroethane | 491.6700 | 11.11 | 0.00 | 240837 | 85.0 | 65.5 | 36.2 | 96.2 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|----------|-------|----------|-------|-------|--------|-------|-------|
| 1,2,3-Trichloropropane | 491.5229 | 11.15 | 0.00 | 64422 | 112.0 | 62.7 | 33.5 | 93.5 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|----------|-------|----------|--------|------|--------|-------|-------|
| 2-Chlorotoluene | 538.4964 | 11.29 | 0.00 | 455991 | 91.0 | 280.4 | 252.3 | 312.3 |






Quantitation Results Report (QT Reviewed)

| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------------|----------|-------|---------------------|---------|-------|--|-------|-------|
| 4-Chlorotoluene | 531.8471 | 11.40 | 0.00 | 1468376 | 126.0 | 31.7 | 1.7 | 61.7 |
| + EIC (91.0) Scan 04JAN21.D | | | 91.0, 126.0 | | | + Scan (11.361-11.453 min, 34 scans) 04JAN21.D | | |
| | | | | | | | | |
| 1,3-Dichlorobenzene | 511.5504 | 12.03 | 0.00 | 793993 | 148.0 | 63.7 | 33.6 | 93.6 |
| + EIC (146.0) Scan 04JAN21.D | | | 146.0, 111.0, 148.0 | | | + Scan (11.991-12.081 min, 33 scans) 04JAN21.D | | |
| | | | | | | | | |
| 1,4-Dichlorobenzene | 502.3001 | 12.13 | 0.00 | 794954 | 148.0 | 63.9 | 33.1 | 93.1 |
| + EIC (146.0) Scan 04JAN21.D | | | 146.0, 111.0, 148.0 | | | + Scan (12.081-12.187 min, 38 scans) 04JAN21.D | | |
| | | | | | | | | |


Quantitation Results Report (QT Reviewed)

| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,2-Dichlorobenzene | 506.3871 | 12.49 | 0.00 | 664247 | 148.0 | 64.3 | 33.9 | 93.9 |
| | | | | | 111.0 | 40.6 | 11.0 | 71.0 |



Quantitation Results Report (QT Reviewed)

| | | | |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File | 04JAN23.D | Operator | MSC |
| Acq. Method | 5975CACQF.M | Acq. Date-Time | 1/4/2022 9:29:14 PM |
| Sample Name | ICV010422 | Instrument | VOA5975C |
| Vial | 23 | Multiplier | 1.00 |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m | Comment | |
| Tune File | BFB_Atune3.u | Tune Date | 10/11/2021 4:02:00 PM |
| Batch Name | VG010422_8260B.batch.bin | Last Calib Update | 1/9/2022 8:59:52 PM |
| Ref Library | \\MASSHUNTER\Org\Library\NIST129K.I | | |



| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|----------|----|------|-------|-------|-------|----------|
|----------|----|------|-------|-------|-------|----------|

Internal Standards

| | | | | | | |
|--------------------------|--------|-------|--------|----------|----|--------|
| M Fluorobenzene | 6.621 | 96.0 | 801210 | 250.0000 | ng | -0.003 |
| M Chlorobenzene-d5 | 9.774 | 82.0 | 307868 | 250.0000 | ng | 0.003 |
| M 1,4-Dichlorobenzene-d4 | 12.100 | 152.0 | 255907 | 250.0000 | ng | 0.000 |

System Monitoring Compounds

| | | | | | | |
|-------------------------|----------------------|-------|--------|--------------------|----|--------|
| S Dibromofluoromethane | 5.848 | 113.0 | 204707 | 271.1994 | ng | 0.003 |
| Spiked Amount: 250.000 | Range: 80.0 - 119.0% | | | Recovery = 108.48% | | |
| S 1,2-Dichloroethane-d4 | 6.230 | 67.0 | 91382 | 280.2886 | ng | -0.003 |
| Spiked Amount: 250.000 | Range: 81.0 - 118.0% | | | Recovery = 112.12% | | |
| S Toluene-d8 | 8.322 | 98.0 | 821531 | 276.9106 | ng | 0.003 |
| Spiked Amount: 250.000 | Range: 89.0 - 112.0% | | | Recovery = 110.76% | | |
| S p-Bromofluorobenzene | 10.951 | 95.0 | 253034 | 269.8976 | ng | -0.003 |
| Spiked Amount: 250.000 | Range: 85.0 - 114.0% | | | Recovery = 107.96% | | |

Target Compounds













| Compound | RT | QIon | Resp. | Conc. | Units | QValue |
|----------------------------------|-------|-------|--------|-----------|-------|--------|
| T Dichlorodifluoromethane | 1.241 | 85.0 | 116936 | 111.3749 | ng | 99 |
| T Chloromethane | 1.406 | 50.0 | 138617 | 108.7739 | ng | 98 |
| T Vinyl chloride | 1.495 | 62.0 | 137775 | 120.1518 | ng | 86 |
| T Bromomethane | 1.796 | 96.0 | 59947 | 116.9157 | ng | 100 |
| T Chloroethane | 1.897 | 64.0 | 65619 | 115.5932 | ng | 99 |
| T Trichlorofluoromethane | 2.145 | 101.0 | 173333 | 121.7847 | ng | 97 |
| T 1,1-Dichloroethene | 2.702 | 96.0 | 108512 | 134.4566 | ng | 100 |
| T Methylene chloride | 3.330 | 49.0 | 144585 | 121.5297 | ng | 98 |
| T trans-1,2-Dichloroethene | 3.715 | 96.0 | 110909 | 134.7028 | ng | 98 |
| T Methyl tert-butyl ether (MTBE) | 3.754 | 73.0 | 143378 | 134.7224 | ng | 99 |
| T 1,1-Dichloroethane | 4.376 | 63.0 | 208131 | 135.8030 | ng | 98 |
| T 2,2-Dichloropropane | 5.190 | 77.0 | 150902 | 131.4031 | ng | 97 |
| T cis-1,2-Dichloroethene | 5.209 | 96.0 | 108623 | 130.1231 | ng | 99 |
| T Methyl ethyl ketone | 5.282 | 43.0 | 135511 | 1198.4439 | ng | 98 |
| T Bromochloromethane | 5.513 | 128.0 | 42744 | 123.6009 | ng | 99 |
| T Chloroform | 5.647 | 83.0 | 183676 | 120.4236 | ng | 100 |

Quantitation Results Report (QT Reviewed)





| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|-----------------------------|--------|-------|--------|----------|-------|----------|
| T 1,1,1-Trichloroethane | 5.831 | 97.0 | 183324 | 128.2524 | ng | 99 |
| T Carbon tetrachloride | 6.027 | 117.0 | 181384 | 128.7928 | ng | 99 |
| T 1,1-Dichloropropene | 6.038 | 75.0 | 150930 | 124.1853 | ng | 100 |
| T Benzene | 6.280 | 78.0 | 418900 | 131.3139 | ng | 99 |
| T 1,2-Dichloroethane | 6.325 | 62.0 | 104249 | 120.7991 | ng | 95 |
| T Trichloroethene | 7.025 | 95.0 | 121734 | 131.1096 | ng | 99 |
| T 1,2-Dichloropropane | 7.270 | 63.0 | 102633 | 125.6626 | ng | 99 |
| T Dibromomethane | 7.393 | 93.0 | 43248 | 125.3047 | ng | 97 |
| T Bromodichloromethane | 7.585 | 83.0 | 122757 | 128.8759 | ng | 100 |
| T cis-1,3-Dichloropropene | 8.054 | 75.0 | 130910 | 121.5561 | ng | 98 |
| T Toluene | 8.386 | 92.0 | 264584 | 132.0244 | ng | 100 |
| T trans-1,3-Dichloropropene | 8.637 | 75.0 | 98907 | 129.0216 | ng | 97 |
| T 1,1,2-Trichloroethane | 8.815 | 83.0 | 49128 | 123.0361 | ng | 98 |
| T Tetrachloroethene | 8.935 | 163.8 | 103027 | 126.0141 | ng | 99 |
| T 1,3-Dichloropropane | 8.980 | 76.0 | 95697 | 121.8442 | ng | 98 |
| T Chlorodibromomethane | 9.203 | 129.0 | 78076 | 125.1103 | ng | 98 |
| T 1,2-Dibromoethane | 9.306 | 107.0 | 54259 | 124.2764 | ng | 100 |
| T Chlorobenzene | 9.802 | 112.0 | 288815 | 131.6352 | ng | 99 |
| T 1,1,1,2-Tetrachloroethane | 9.892 | 131.0 | 97148 | 126.6657 | ng | 95 |
| T Ethylbenzene | 9.917 | 91.0 | 501953 | 131.9113 | ng | 99 |
| T m+p-Xylenes | 10.039 | 106.0 | 388558 | 262.7589 | ng | 100 |
| T o-Xylene | 10.430 | 106.0 | 174061 | 132.2214 | ng | 98 |
| T Styrene | 10.449 | 104.0 | 291425 | 137.4974 | ng | 98 |
| T Bromoform | 10.628 | 172.5 | 42560 | 129.9644 | ng | 98 |
| T Bromobenzene | 11.093 | 156.0 | 109054 | 131.6788 | ng | 99 |
| T 1,1,2,2-Tetrachloroethane | 11.113 | 83.0 | 60763 | 127.4722 | ng | 98 |
| T 1,2,3-Trichloropropane | 11.146 | 110.0 | 15682 | 122.9523 | ng | 99 |
| T 2-Chlorotoluene | 11.291 | 126.0 | 108192 | 131.2948 | ng | 95 |
| T 4-Chlorotoluene | 11.400 | 91.0 | 368295 | 137.0790 | ng | 100 |
| T 1,3-Dichlorobenzene | 12.033 | 146.0 | 204088 | 135.1185 | ng | 99 |
| T 1,4-Dichlorobenzene | 12.122 | 146.0 | 200032 | 129.8812 | ng | 99 |
| T 1,2-Dichlorobenzene | 12.493 | 146.0 | 164299 | 128.7104 | ng | 99 |

(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)

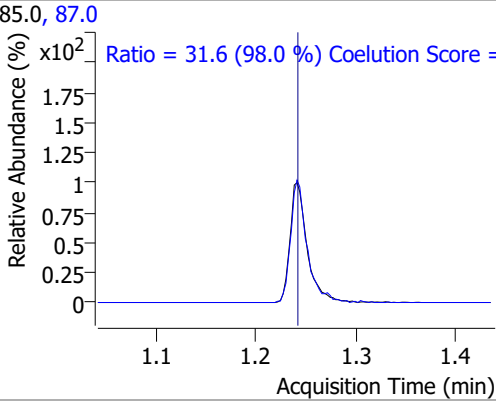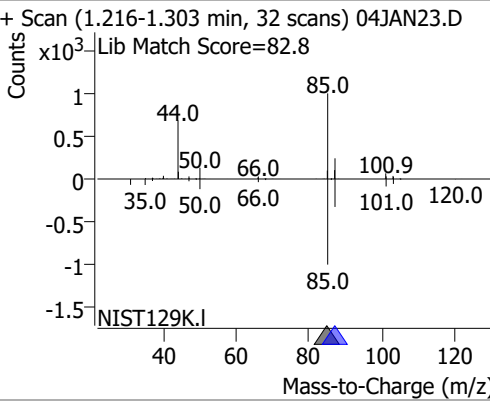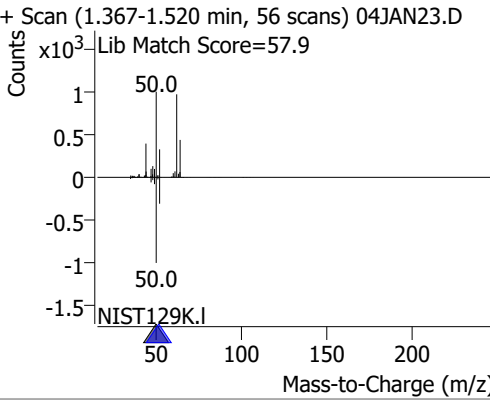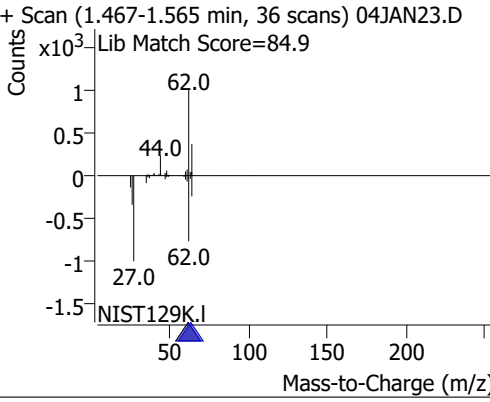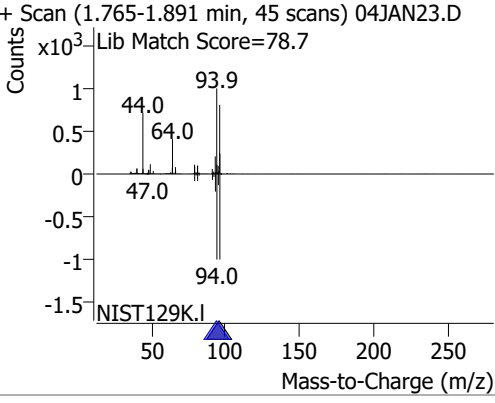
| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--|--|------|---|--------|------|--|-------|-------|
| Dichlorodifluoromethane | 111.3749 | 1.24 | 0.00 | 116936 | 87.0 | 31.6 | 2.3 | 62.3 |
| + EIC (85.0) Scan 04JAN23.D | | | 85.0, 87.0 | | | + Scan (1.216-1.303 min, 32 scans) 04JAN23.D | | |
|  |  | |  | | | | | |
| Chloromethane | 108.7739 | 1.41 | 0.00 | 138617 | 52.0 | 33.2 | 2.1 | 62.1 |
| + EIC (50.0) Scan 04JAN23.D | | | 50.0, 52.0 | | | + Scan (1.367-1.520 min, 56 scans) 04JAN23.D | | |
|  |  | |  | | | | | |
| Vinyl chloride | 120.1518 | 1.49 | 0.00 | 137775 | 64.0 | 37.7 | 0.0 | 59.9 |
| + EIC (62.0) Scan 04JAN23.D | | | 62.0, 64.0 | | | + Scan (1.467-1.565 min, 36 scans) 04JAN23.D | | |
|  |  | |  | | | | | |
| Bromomethane | 116.9157 | 1.80 | 0.00 | 59947 | 94.0 | 105.0 | 74.6 | 134.6 |
| + EIC (96.0) Scan 04JAN23.D | | | 96.0, 94.0 | | | + Scan (1.765-1.891 min, 45 scans) 04JAN23.D | | |
|  |  | |  | | | | | |

Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------------|----------|------|----------|--------|------|--------|-------|-------|
| trans-1,2-Dichloroethene | 134.7028 | 3.71 | 0.00 | 110909 | 61.0 | 156.1 | 123.9 | 183.9 |
| | | | | | 98.0 | 64.1 | 35.7 | 95.7 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------------------|----------|------|----------|--------|------|--------|-------|-------|
| Methyl tert-butyl ether (MTBE) | 134.7224 | 3.75 | 0.00 | 143378 | 57.0 | 25.1 | 0.0 | 54.6 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1-Dichloroethane | 135.8030 | 4.38 | 0.00 | 208131 | 65.0 | 31.2 | 2.1 | 62.1 |
| | | | | | 83.0 | 12.9 | 0.0 | 43.7 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 2,2-Dichloropropane | 131.4031 | 5.19 | -0.01 | 150902 | 41.0 | 63.6 | 36.5 | 96.5 |
| | | | | | 97.0 | 22.5 | 0.0 | 53.2 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,2-Dichloroethene | 130.1231 | 5.21 | -0.01 | 108623 | 61.0 | 168.1 | 137.2 | 197.2 |
| | | | | | 98.0 | 67.7 | 37.3 | 97.3 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|-----------|------|----------|--------|------|--------|-------|-------|
| Methyl ethyl ketone | 1198.4439 | 5.28 | 0.00 | 135511 | 72.0 | 20.4 | 0.0 | 51.3 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|-------|------|--------|-------|-------|
| Bromochloromethane | 123.6009 | 5.51 | -0.01 | 42744 | 49.0 | 184.6 | 152.9 | 212.9 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|------|--------|-------|-------|
| Chloroform | 120.4236 | 5.65 | -0.01 | 183676 | 85.0 | 66.1 | 36.0 | 96.0 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1,1-Trichloroethane | 128.2524 | 5.83 | 0.00 | 183324 | 99.0 | 65.1 | 34.7 | 94.7 |
| | | | | | 61.0 | 48.9 | 18.1 | 78.1 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Dibromofluoromethane | 271.1994 | 5.85 | 0.00 | 204707 | 191.5 | 22.0 | 0.0 | 53.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Carbon tetrachloride | 128.7928 | 6.03 | 0.00 | 181384 | 119.0 | 96.4 | 67.2 | 127.2 |
| | | | | | 121.0 | 30.9 | 0.1 | 60.1 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|-------|--------|-------|-------|
| 1,1-Dichloropropene | 124.1853 | 6.04 | 0.00 | 150930 | 110.0 | 36.1 | 5.9 | 65.9 |
| | | | | | 77.0 | 30.4 | 0.1 | 60.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 280.2886 | 6.23 | 0.00 | 91382 | 65.0 | 194.9 | 166.5 | 226.5 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|------|----------|--------|------|--------|-------|-------|
| Benzene | 131.3139 | 6.28 | 0.00 | 418900 | 77.0 | 23.2 | 0.0 | 53.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloroethane | 120.7991 | 6.32 | 0.00 | 104249 | 64.0 | 33.3 | 0.0 | 59.9 |
| | | | | | 98.0 | 8.1 | 0.0 | 37.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|----------|------|----------|--------|-------|--------|-------|-------|
| Trichloroethene | 131.1096 | 7.02 | -0.01 | 121734 | 130.0 | 102.3 | 71.5 | 131.5 |
| | | | | | 97.0 | 63.0 | 34.1 | 94.1 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloropropane | 125.6626 | 7.27 | 0.00 | 102633 | 76.0 | 37.9 | 8.2 | 68.2 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------|----------|------|----------|-------|-------|--------|-------|-------|
| Dibromomethane | 125.3047 | 7.39 | -0.01 | 43248 | 173.5 | 109.3 | 83.7 | 143.7 |
| | | | | | 95.0 | 81.2 | 52.2 | 112.2 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Bromodichloromethane | 128.8759 | 7.59 | 0.00 | 122757 | 85.0 | 64.3 | 34.5 | 94.5 |
| | | | | | 127.0 | 9.3 | 0.0 | 39.6 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,3-Dichloropropene | 121.5561 | 8.05 | -0.01 | 130910 | 39.0 | 51.6 | 23.3 | 83.3 |
| | | | | | 77.0 | 31.2 | 1.0 | 61.0 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 276.9106 | 8.32 | 0.00 | 821531 | 100.0 | 64.3 | 34.4 | 94.4 |
| | | | | | 99.0 | 9.6 | 0.0 | 39.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|------|----------|--------|------|--------|-------|-------|
| Toluene | 132.0244 | 8.39 | 0.00 | 264584 | 91.0 | 175.5 | 145.8 | 205.8 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|----------|------|----------|-------|------|--------|-------|-------|
| trans-1,3-Dichloropropene | 129.0216 | 8.64 | 0.00 | 98907 | 39.0 | 50.5 | 23.4 | 83.4 |
| | | | | | 77.0 | 31.0 | 2.4 | 62.4 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,1,2-Trichloroethane | 123.0361 | 8.82 | 0.00 | 49128 | 97.0 | 115.4 | 84.6 | 144.6 |
| | | | | | 85.0 | 64.6 | 37.6 | 97.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Tetrachloroethene | 126.0141 | 8.94 | 0.00 | 103027 | 165.8 | 130.8 | 98.6 | 158.6 |
| | | | | | 129.0 | 91.8 | 61.5 | 121.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,3-Dichloropropane | 121.8442 | 8.98 | 0.00 | 95697 | 78.0 | 32.1 | 2.9 | 62.9 |







| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|-------|-------|--------|-------|-------|
| Chlorodibromomethane | 125.1103 | 9.20 | 0.00 | 78076 | 127.0 | 76.5 | 48.0 | 108.0 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------|----------|------|----------|-------|-------|--------|-------|-------|
| 1,2-Dibromoethane | 124.2764 | 9.31 | 0.00 | 54259 | 109.0 | 94.9 | 64.5 | 124.5 |




Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|-------|----------|--------|------|--------|-------|-------|
| o-Xylene | 132.2214 | 10.43 | 0.00 | 174061 | 91.0 | 215.8 | 183.1 | 243.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|-------|----------|--------|------|--------|-------|-------|
| Styrene | 137.4974 | 10.45 | 0.00 | 291425 | 78.0 | 48.1 | 19.6 | 79.6 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------|----------|-------|----------|-------|----------------|--------------|--------------|--------------|
| Bromoform | 129.9644 | 10.63 | 0.00 | 42560 | 170.5 174.5 | 50.3 49.3 | 22.1 20.1 | 82.1 80.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|----------------|--------------|--------------|----------------|
| p-Bromofluorobenzene | 269.8976 | 10.95 | 0.00 | 253034 | 174.0 176.0 | 93.4 90.2 | 61.7 60.6 | 121.7 120.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|----------|-------|----------|--------|-------|--------|-------|-------|
| Bromobenzene | 131.6788 | 11.09 | 0.00 | 109054 | 77.0 | 146.1 | 115.7 | 175.7 |
| | | | | | 158.0 | 99.0 | 66.5 | 126.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|----------|-------|----------|-------|------|--------|-------|-------|
| 1,1,2,2-Tetrachloroethane | 127.4722 | 11.11 | 0.00 | 60763 | 85.0 | 64.8 | 36.2 | 96.2 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|----------|-------|----------|-------|-------|--------|-------|-------|
| 1,2,3-Trichloropropane | 122.9523 | 11.15 | 0.00 | 15682 | 112.0 | 62.6 | 33.5 | 93.5 |






| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|----------|-------|----------|--------|------|--------|-------|-------|
| 2-Chlorotoluene | 131.2948 | 11.29 | 0.00 | 108192 | 91.0 | 290.9 | 252.3 | 312.3 |






Quantitation Results Report (QT Reviewed)




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 4-Chlorotoluene | 137.0790 | 11.40 | 0.00 | 368295 | 126.0 | 31.8 | 1.7 | 61.7 |



| | | | | | | | | |
|---------------------|----------|-------|------|--------|-------|------|------|------|
| 1,3-Dichlorobenzene | 135.1185 | 12.03 | 0.00 | 204088 | 148.0 | 63.2 | 33.6 | 93.6 |
| | | | | | 111.0 | 38.4 | 9.8 | 69.8 |






| | | | | | | | | |
|---------------------|----------|-------|------|--------|-------|------|------|------|
| 1,4-Dichlorobenzene | 129.8812 | 12.12 | 0.00 | 200032 | 148.0 | 63.9 | 33.1 | 93.1 |
| | | | | | 111.0 | 39.1 | 9.1 | 69.1 |



Quantitation Results Report (QT Reviewed)

| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,2-Dichlorobenzene | 128.7104 | 12.49 | 0.00 | 164299 | 148.0 | 64.3 | 33.9 | 93.9 |
| | | | | | 111.0 | 40.6 | 11.0 | 71.0 |



Audit Trail report

Batch name and path: D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin
Quant batch version: 10.0
Quant reporting version: 10.0

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|------------------------------|----------------|----------------------|---|--------|---------|---------|-----------|
| CmdNewBatchTable | BL2000\mchavez | 1/4/2022 10:36:43 AM | Create new batch D:\Org\Data\VOA5975C\VG010422\VG010422_8260B.batch.bin | | | ✓ | |
| CmdImportSamplesFromWorklist | BL2000\mchavez | 1/4/2022 10:36:56 AM | Add samples from worklist: D:\Org\Data\VOA5975C\VG010422\04JAN02.D, D:\Org\Data\VOA5975C\VG010422\04JAN01.D | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/4/2022 10:37:01 AM | Set SampleType = MatrixBlank for sample 04JAN02.D; previous value = Sample | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/4/2022 10:37:04 AM | Set SampleType = TuneCheck for sample 04JAN02.D; previous value = MatrixBlank | | | ✓ | |
| CmdStartMethodEditing | BL2000\mchavez | 1/4/2022 10:52:58 AM | Start method editing | | | ✓ | |
| CmdImportMethodFromBatch | BL2000\mchavez | 1/4/2022 10:52:59 AM | Import method from batch D:\Org\Data\VOA5975C\VG010322\VG010322_8260B_2ndRun.batch.bin | | | ✓ | |
| CmdApplyMethodToAllSamples | BL2000\mchavez | 1/4/2022 10:53:03 AM | Apply method to all samples | | | ✓ | |
| CmdMethodClear | BL2000\mchavez | 1/4/2022 10:53:03 AM | Clear method | | | ✓ | |
| CmdEndMethodEditing | BL2000\mchavez | 1/4/2022 10:53:03 AM | End method editing | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/4/2022 10:53:07 AM | Quantitate all compounds in all samples | | | ✓ | |
| CmdSaveBatchTable | BL2000\mchavez | 1/4/2022 10:54:55 AM | Save batch D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | | | ✓ | |
| CmdOpenBatchTable | BL2000\mchavez | 1/4/2022 11:14:07 AM | Open batch D:\Org\Data\VOA5975C\VG010422\VG010422_8260B.batch.bin | | | ✓ | |
| CmdImportSamplesFromWorklist | BL2000\mchavez | 1/4/2022 11:14:24 AM | Add samples from worklist: D:\Org\Data\VOA5975C\VG010422\04JAN03.D | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/4/2022 11:14:28 AM | Set SampleType = CC for sample 04JAN03.D; previous value = Sample | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/4/2022 11:14:31 AM | Set LevelName = CC for sample 04JAN03.D; previous value = | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/4/2022 11:14:35 AM | Quantitate all compounds in all samples | | | ✓ | |
| CmdSaveBatchTable | BL2000\mchavez | 1/4/2022 11:15:38 AM | Save batch D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | | | ✓ | |
| CmdOpenBatchTable | BL2000\mchavez | 1/4/2022 1:02:39 PM | Open batch D:\Org\Data\VOA5975C\VG010422\VG010422_8260B.batch.bin | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|------------------------------|----------------|---------------------|---|--------|---------|---------|-----------|
| CmdImportSamplesFromWorklist | BL2000\mchavez | 1/4/2022 1:02:58 PM | Add samples from worklist: D:\Org\Data\VOA5975C\VG010422\04JAN05.D, D:\Org\Data\VOA5975C\VG010422\04JAN04.D | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/4/2022 1:03:09 PM | Set SampleType = TuneCheck for sample 04JAN05.D; previous value = Sample | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/4/2022 1:03:40 PM | Quantitate all compounds in all samples | | | ✓ | |
| CmdSaveBatchTable | BL2000\mchavez | 1/4/2022 1:14:26 PM | Save batch D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | | | ✓ | |
| CmdOpenBatchTable | BL2000\mchavez | 1/4/2022 1:47:13 PM | Open batch D:\Org\Data\VOA5975C\VG010422\VG010422_8260B.batch.bin | | | ✓ | |
| CmdImportSamplesFromWorklist | BL2000\mchavez | 1/4/2022 1:47:29 PM | Add samples from worklist: D:\Org\Data\VOA5975C\VG010422\04JAN06.D | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/4/2022 1:47:35 PM | Set SampleType = CC for sample 04JAN06.D; previous value = Sample | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/4/2022 1:47:38 PM | Set LevelName = CC for sample 04JAN06.D; previous value = | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/4/2022 1:47:44 PM | Quantitate all compounds in all samples | | | ✓ | |
| CmdSaveBatchTable | BL2000\mchavez | 1/4/2022 1:53:45 PM | Save batch D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | | | ✓ | |
| CmdOpenBatchTable | BL2000\mchavez | 1/4/2022 3:05:35 PM | Open batch D:\Org\Data\VOA5975C\VG010422\VG010422_8260B.batch.bin | | | ✓ | |
| CmdImportSamplesFromWorklist | BL2000\mchavez | 1/4/2022 3:06:14 PM | Add samples from worklist: D:\Org\Data\VOA5975C\VG010422\04JAN08.D, D:\Org\Data\VOA5975C\VG010422\04JAN07.D | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/4/2022 3:06:26 PM | Set SampleType = TuneCheck for sample 04JAN08.D; previous value = Sample | | | ✓ | |
| CmdSaveBatchTable | BL2000\mchavez | 1/4/2022 3:24:14 PM | Save batch D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | | | ✓ | |
| CmdOpenBatchTable | BL2000\mchavez | 1/5/2022 8:56:03 AM | Open batch D:\Org\Data\VOA5975C\VG010422\VG010422_8260B.batch.bin | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|------------------------------|----------------|---------------------|---|--------|---------|---------|-----------|
| CmdImportSamplesFromWorklist | BL2000\mchavez | 1/5/2022 8:58:43 AM | Add samples from worklist: D:\Org\Data\VOA5975C\VG010422\04JAN28.D, D:\Org\Data\VOA5975C\VG010422\04JAN27.D, D:\Org\Data\VOA5975C\VG010422\04JAN26.D, D:\Org\Data\VOA5975C\VG010422\04JAN25.D, D:\Org\Data\VOA5975C\VG010422\04JAN24.D, D:\Org\Data\VOA5975C\VG010422\04JAN23.D, D:\Org\Data\VOA5975C\VG010422\04JAN22.D, D:\Org\Data\VOA5975C\VG010422\04JAN21.D, D:\Org\Data\VOA5975C\VG010422\04JAN20.D, D:\Org\Data\VOA5975C\VG010422\04JAN19.D, D:\Org\Data\VOA5975C\VG010422\04JAN18.D, D:\Org\Data\VOA5975C\VG010422\04JAN17.D, D:\Org\Data\VOA5975C\VG010422\04JAN16.D, D:\Org\Data\VOA5975C\VG010422\04JAN15.D, D:\Org\Data\VOA5975C\VG010422\04JAN14.D, D:\Org\Data\VOA5975C\VG010422\04JAN13.D, D:\Org\Data\VOA5975C\VG010422\04JAN12.D, D:\Org\Data\VOA5975C\VG010422\04JAN11.D, D:\Org\Data\VOA5975C\VG010422\04JAN10.D, D:\Org\Data\VOA5975C\VG010422\04JAN09.D | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 8:59:26 AM | Set SampleType = Blank for sample 04JAN09.D; previous value = Sample | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 8:59:31 AM | Set SampleType = Calibration for sample 04JAN10.D; previous value = Sample | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 8:59:35 AM | Set SampleType = Calibration for sample 04JAN11.D; previous value = Sample | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 8:59:40 AM | Set SampleType = Calibration for sample 04JAN12.D; previous value = Sample | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 8:59:45 AM | Set SampleType = Calibration for sample 04JAN13.D; previous value = Sample | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------|----------------|---------------------|---|--------|---------|---------|--|
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 8:59:50 AM | Set SampleType = Calibration for sample 04JAN15.D; previous value = Sample | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 8:59:55 AM | Set SampleType = Calibration for sample 04JAN17.D; previous value = Sample | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 9:00:00 AM | Set SampleType = Calibration for sample 04JAN19.D; previous value = Sample | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 9:00:08 AM | Set SampleType = Calibration for sample 04JAN21.D; previous value = Sample | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 9:00:14 AM | Set SampleType = QC for sample 04JAN23.D; previous value = Sample | | | ✓ | |
| CmdSaveBatchTable | BL2000\mchavez | 1/5/2022 9:11:16 AM | Save batch D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | | | ✓ | |
| CmdOpenBatchTable | BL2000\mchavez | 1/5/2022 9:58:34 AM | Open batch D:\Org\Data\VOA5975C\VG010422\VG010422_8260B.batch.bin | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/5/2022 9:58:40 AM | Quantitate all compounds in all samples | | | | Agilent.MassSpectrometry.DataAnalysis.Quantitative.ApplicationCommandException: Batch quantitation failed ---> Agilent.MassSpectrometry.DataAnalysis.Quantitative.ApplicationCommandException: Sample not validated: Level name is undefined for a Calibration or QC sample. at Agilent.MassSpectrometry.DataAnalysis.Quantitative.Analysis.Batch.ValidateBatchMethod() at Agilent.MassSpectrometry.DataAnalysis.Quantitative.Analysis.Batch.Quantitate() --- End of inner exception stack trace --- at Agilent.MassSpectrometry.DataAnalysis.Quantitative.Analysis.Batch.Quantitate() at Agilent.MassSpectrometry.DataAnalysis.Quantitative.CmdQuantitate.QuantitateBatch(Int16 batchId) at Agilent.MassSpectrometry.CommandModel.CommandHistory.Invoke(ICommand cmd) at Agilent.MassSpectrometry.DataAnalysis.Quantitative.AppCommandContext.Invoke(ICommand cmd) |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|---|--------|---------|---------|-----------|
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 10:06:05 AM | Set LevelName = 1 for sample 04JAN10.D; previous value = | | | ✓ | |
| CmdSaveBatchTable | BL2000\mchavez | 1/5/2022 10:06:09 AM | Save batch D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | | | ✓ | |
| CmdOpenBatchTable | BL2000\mchavez | 1/5/2022 10:14:38 AM | Open batch D:\Org\Data\VOA5975C\VG010422\VG010422_8260B.batch.bin | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 10:14:47 AM | Set LevelName = 2 for sample 04JAN11.D; previous value = | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 10:14:52 AM | Set LevelName = 3 for sample 04JAN12.D; previous value = | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 10:14:57 AM | Set LevelName = 4 for sample 04JAN13.D; previous value = | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 10:15:05 AM | Set LevelName = 5 for sample 04JAN15.D; previous value = | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 10:15:11 AM | Set LevelName = 6 for sample 04JAN17.D; previous value = | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 10:15:16 AM | Set LevelName = 7 for sample 04JAN19.D; previous value = | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 10:15:21 AM | Set LevelName = 8 for sample 04JAN21.D; previous value = | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 10:15:29 AM | Set LevelName = QC for sample 04JAN23.D; previous value = | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 10:15:36 AM | Set SampleInformation = LCSA for sample 04JAN23.D; previous value = | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/5/2022 10:16:01 AM | Quantitate all compounds in all samples | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 10:16:49 AM | Manually integrate compound Chloroethane in sample 04JAN10.D, from x, y = 1.874, 1384 to 1.916, 1542, result = 2178; previous integration is from x, y = 1.894, 1143 to 1.933, 1143 and previous response = 2132. | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:16:53 AM | Manually integrate qualifier 66.0 of compound Chloroethane in sample 04JAN10.D from x, y = 1.869, 0 to 1.908, 8; result = 781 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:16:54 AM | Manually integrate qualifier 66.0 of compound Chloroethane in sample 04JAN10.D, from x, y = 1.869, 0 to 1.913, 0, result = 824; previous integration is from x, y = 1.869, 0 to 1.908, 8 and previous response = 781. | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 10:17:08 AM | Manually integrate compound Bromomethane in sample 04JAN10.D from x, y = 1.768, -2 to 1.849, 0; result = 1902 | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|---|--------|---------|---------|-----------|
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:17:15 AM | Manually integrate qualifier 87.0 of compound Dichlorodifluoromethane in sample 04JAN10.D from x, y = 1.202, 0 to 1.289, 0; result = 1393 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:17:25 AM | Manually integrate qualifier 52.0 of compound Chloromethane in sample 04JAN10.D from x, y = 1.370, 0 to 1.459, 0; result = 1679 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:17:55 AM | Manually integrate qualifier 64.0 of compound Vinyl chloride in sample 04JAN10.D, from x, y = 1.492, 6362 to 1.506, 5900, result = 1131; previous integration is from x, y = 1.308, 0 to 1.682, 0 and previous response = 192320. | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 10:18:11 AM | Manually integrate compound 1,1-Dichloroethene in sample 04JAN10.D from x, y = 2.636, 0 to 2.747, 0; result = 2084 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:18:16 AM | Manually integrate qualifier 63.0 of compound 1,1-Dichloroethene in sample 04JAN10.D from x, y = 2.672, 0 to 2.753, 0; result = 1158 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:18:38 AM | Manually integrate qualifier 86.0 of compound Methylene chloride in sample 04JAN10.D from x, y = 3.288, 0 to 3.386, 0; result = 1820 | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 10:19:27 AM | Manually integrate compound trans-1,2-Dichloroethene in sample 04JAN10.D from x, y = 3.673, 0 to 3.762, 0; result = 2146 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:19:31 AM | Manually integrate qualifier 98.0 of compound trans-1,2-Dichloroethene in sample 04JAN10.D from x, y = 3.684, 0 to 3.779, 0; result = 1426 | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 10:19:36 AM | Manually integrate compound Methyl tert-butyl ether (MTBE) in sample 04JAN10.D from x, y = 3.698, 0 to 3.832, 0; result = 2717 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:19:38 AM | Manually integrate qualifier 57.0 of compound Methyl tert-butyl ether (MTBE) in sample 04JAN10.D from x, y = 3.690, 0 to 3.798, 0; result = 531 | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 10:19:46 AM | Manually integrate compound 2,2-Dichloropropane in sample 04JAN10.D from x, y = 5.137, 0 to 5.279, 0; result = 2930 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:19:49 AM | Manually integrate qualifier 97.0 of compound 2,2-Dichloropropane in sample 04JAN10.D from x, y = 5.151, 0 to 5.285, 0; result = 814 | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|---|--------|---------|---------|-----------|
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:19:52 AM | Manually integrate qualifier41.0 of compound 2,2-Dichloropropane in sample 04JAN10.D from x, y = 5.151, 0 to 5.257, 0; result = 2246 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:20:11 AM | Manually integrate qualifier65.0 of compound 1,1-Dichloroethane in sample 04JAN10.D from x, y = 4.323, 0 to 4.465, 0; result = 1347 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:20:13 AM | Manually integrate qualifier83.0 of compound 1,1-Dichloroethane in sample 04JAN10.D from x, y = 4.342, 0 to 4.426, 0; result = 227 | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 10:26:02 AM | Manually integrate compound cis-1,2-Dichloroethene in sample 04JAN10.D from x, y = 5.145, 0 to 5.282, 0; result = 2376 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:26:05 AM | Manually integrate qualifier61.0 of compound cis-1,2-Dichloroethene in sample 04JAN10.D from x, y = 5.151, 0 to 5.274, 0; result = 4139 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:26:07 AM | Manually integrate qualifier98.0 of compound cis-1,2-Dichloroethene in sample 04JAN10.D from x, y = 5.176, 0 to 5.257, 0; result = 1525 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:26:12 AM | Manually integrate qualifier72.0 of compound Methyl ethyl ketone in sample 04JAN10.D from x, y = 5.274, 0 to 5.343, 0; result = 435 | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 10:26:18 AM | Manually integrate compound Bromochloromethane in sample 04JAN10.D from x, y = 5.463, 0 to 5.555, 0; result = 807 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:26:20 AM | Manually integrate qualifier49.0 of compound Bromochloromethane in sample 04JAN10.D from x, y = 5.472, 0 to 5.558, 0; result = 1686 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:26:23 AM | Manually integrate qualifier85.0 of compound Chloroform in sample 04JAN10.D from x, y = 5.592, 0 to 5.734, 0; result = 2708 | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 10:26:28 AM | Manually integrate compound Dibromofluoromethane in sample 04JAN10.D from x, y = 5.812, 0 to 5.915, 0; result = 2508 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:26:30 AM | Manually integrate qualifier191.5 of compound Dibromofluoromethane in sample 04JAN10.D from x, y = 5.809, 0 to 5.884, 0; result = 479 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:26:37 AM | Manually integrate qualifier61.0 of compound 1,1,1-Trichloroethane in sample 04JAN10.D from x, y = 5.790, 0 to 5.890, 0; result = 1705 | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|---|--------|---------|---------|-----------|
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:26:42 AM | Manually integrate qualifier121.0 of compound Carbon tetrachloride in sample 04JAN10.D from x, y = 5.999, 0 to 6.068, 0; result = 903 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:26:46 AM | Manually integrate qualifier110.0 of compound 1,1-Dichloropropene in sample 04JAN10.D from x, y = 5.993, 0 to 6.074, 0; result = 1122 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:26:48 AM | Manually integrate qualifier77.0 of compound 1,1-Dichloropropene in sample 04JAN10.D from x, y = 6.013, 0 to 6.099, 0; result = 1052 | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 10:26:53 AM | Manually integrate compound 1,2-Dichloroethane-d4 in sample 04JAN10.D from x, y = 6.188, -35 to 6.283, 0; result = 1023 | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 10:26:58 AM | Manually integrate compound 1,2-Dichloroethane-d4 in sample 04JAN10.D, from x, y = 6.197, 0 to 6.283, 0, result = 923; previous integration is from x, y = 6.188, -35 to 6.283, 0 and previous response = 1023. | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:27:00 AM | Manually integrate qualifier65.0 of compound 1,2-Dichloroethane-d4 in sample 04JAN10.D from x, y = 6.199, 0 to 6.275, 0; result = 1927 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:27:34 AM | Manually integrate qualifier77.0 of compound Benzene in sample 04JAN10.D from x, y = 6.222, 0 to 6.339, 0; result = 1884 | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 10:27:39 AM | Manually integrate compound 1,2-Dichloroethane in sample 04JAN10.D from x, y = 6.269, 0 to 6.386, 0; result = 2415 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:27:41 AM | Manually integrate qualifier64.0 of compound 1,2-Dichloroethane in sample 04JAN10.D from x, y = 6.280, 0 to 6.378, 0; result = 761 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:27:43 AM | Manually integrate qualifier98.0 of compound 1,2-Dichloroethane in sample 04JAN10.D from x, y = 6.303, 0 to 6.386, 0; result = 119 | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 10:27:47 AM | Manually integrate compound Trichloroethene in sample 04JAN10.D from x, y = 6.989, 0 to 7.083, 0; result = 2372 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:27:51 AM | Manually integrate qualifier 130.0 of compound Trichloroethene in sample 04JAN10.D, from x, y = 6.997, 0 to 7.072, 0, result = 2567; previous integration is from x, y = 6.997, 0 to 7.044, 0 and previous response = 2405. | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|---|--------|---------|---------|-----------|
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:27:53 AM | Manually integrate qualifier 97.0 of compound Trichloroethene in sample 04JAN10.D from x, y = 6.991, 0 to 7.078, 0; result = 1659 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:27:59 AM | Manually integrate qualifier 76.0 of compound 1,2-Dichloropropane in sample 04JAN10.D from x, y = 7.231, 0 to 7.321, 0; result = 733 | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 10:28:03 AM | Manually integrate compound Dibromomethane in sample 04JAN10.D from x, y = 7.357, 0 to 7.424, 0; result = 902 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:28:06 AM | Manually integrate qualifier 95.0 of compound Dibromomethane in sample 04JAN10.D from x, y = 7.357, 0 to 7.454, 0; result = 535 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:28:09 AM | Manually integrate qualifier 173.5 of compound Dibromomethane in sample 04JAN10.D from x, y = 7.360, 0 to 7.429, 0; result = 1002 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:28:15 AM | Manually integrate qualifier 85.0 of compound Bromodichloromethane in sample 04JAN10.D from x, y = 7.546, 0 to 7.633, 0; result = 1631 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:28:17 AM | Manually integrate qualifier 127.0 of compound Bromodichloromethane in sample 04JAN10.D from x, y = 7.569, 0 to 7.633, 0; result = 130 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:28:23 AM | Manually integrate qualifier 77.0 of compound cis-1,3-Dichloropropene in sample 04JAN10.D from x, y = 8.009, 0 to 8.107, 0; result = 922 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:28:35 AM | Manually integrate qualifier 39.0 of compound cis-1,3-Dichloropropene in sample 04JAN10.D from x, y = 8.037, 0 to 8.090, 0; result = 1459 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:28:40 AM | Manually integrate qualifier 99.0 of compound Toluene-d8 in sample 04JAN10.D from x, y = 8.271, 0 to 8.350, 0; result = 699 | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 10:28:47 AM | Manually integrate compound trans-1,3-Dichloropropene in sample 04JAN10.D from x, y = 8.614, 0 to 8.684, 0; result = 1470 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:28:50 AM | Manually integrate qualifier 77.0 of compound trans-1,3-Dichloropropene in sample 04JAN10.D, from x, y = 8.601, 0 to 8.656, -10, result = 8023; previous integration is from x, y = 8.656, 57 to 8.709, 135 and previous response = 3575. | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|--|--------|---------|---------|-----------|
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:29:03 AM | Manually integrate qualifier 77.0 of compound trans-1,3-Dichloropropene in sample 04JAN10.D, from x, y = 8.601, 0 to 8.656, 156, result = 6858; previous integration is from x, y = 8.601, 0 to 8.835, -10 and previous response = 8023. | | | ✓ | |
| CmdManuallyIntegrateDropBaseline | BL2000\mchavez | 1/5/2022 10:29:04 AM | Drop baseline for qualifier 77.0 of compound trans-1,3-Dichloropropene in sample 04JAN10.D to y = 0, new integration is from x, y = 8.601, 0 to 8.835, 0 and new response = 7954; previous integration is from x, y = 8.601, 0 to 8.835, 156 and previous response = 6858. | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:29:09 AM | Manually integrate qualifier 77.0 of compound trans-1,3-Dichloropropene in sample 04JAN10.D, from x, y = 8.601, 0 to 8.648, 141, result = 368; previous integration is from x, y = 8.601, 0 to 8.835, 0 and previous response = 7954. | | | ✓ | |
| CmdManuallyIntegrateDropBaseline | BL2000\mchavez | 1/5/2022 10:29:12 AM | Drop baseline for qualifier 77.0 of compound trans-1,3-Dichloropropene in sample 04JAN10.D to y = 0, new integration is from x, y = 8.601, 0 to 8.648, 0 and new response = 568; previous integration is from x, y = 8.601, 0 to 8.648, 141 and previous response = 368. | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:29:19 AM | Manually integrate qualifier 39.0 of compound trans-1,3-Dichloropropene in sample 04JAN10.D from x, y = 8.614, 0 to 8.648, 26; result = 974 | | | ✓ | |
| CmdManuallyIntegrateDropBaseline | BL2000\mchavez | 1/5/2022 10:29:21 AM | Drop baseline for qualifier 39.0 of compound trans-1,3-Dichloropropene in sample 04JAN10.D to y = 0, new integration is from x, y = 8.614, 0 to 8.648, 0 and new response = 1000; previous integration is from x, y = 8.614, 0 to 8.648, 26 and previous response = 974. | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 10:29:29 AM | Manually integrate compound 1,1,2-Trichloroethane in sample 04JAN10.D from x, y = 8.785, 0 to 8.843, 0; result = 960 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:29:31 AM | Manually integrate qualifier 97.0 of compound 1,1,2-Trichloroethane in sample 04JAN10.D from x, y = 8.782, 0 to 8.857, 0; result = 1099 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:29:34 AM | Manually integrate qualifier 85.0 of compound 1,1,2-Trichloroethane in sample 04JAN10.D from x, y = 8.796, 0 to 8.851, 0; result = 418 | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|--|--------|---------|---------|-----------|
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 10:29:39 AM | Manually integrate compound Tetrachloroethene in sample 04JAN10.D from x, y = 8.899, 0 to 8.983, 0; result = 2105 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:29:43 AM | Manually integrate qualifier 165.8 of compound Tetrachloroethene in sample 04JAN10.D from x, y = 8.885, 0 to 9.019, 0; result = 2853 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:29:48 AM | Manually integrate qualifier 78.0 of compound 1,3-Dichloropropane in sample 04JAN10.D from x, y = 8.952, 0 to 9.010, 0; result = 452 | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 10:29:52 AM | Manually integrate compound Chlorodibromomethane in sample 04JAN10.D from x, y = 9.169, 0 to 9.256, 0; result = 1468 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:29:54 AM | Manually integrate qualifier 127.0 of compound Chlorodibromomethane in sample 04JAN10.D from x, y = 9.175, 0 to 9.242, 0; result = 1140 | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 10:29:58 AM | Manually integrate compound 1,2-Dibromoethane in sample 04JAN10.D from x, y = 9.278, 0 to 9.348, 0; result = 1299 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:30:00 AM | Manually integrate qualifier 109.0 of compound 1,2-Dibromoethane in sample 04JAN10.D from x, y = 9.275, 0 to 9.340, 0; result = 1039 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:30:35 AM | Manually integrate qualifier 64.0 of compound Vinyl chloride in sample 04JAN15.D, from x, y = 1.476, 4348 to 1.540, 3059, result = 44384; previous integration is from x, y = 1.478, 954 to 1.687, 2147 and previous response = 61198. | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 10:35:03 AM | Set SampleApproved = True for sample 04JAN15.D; previous value = False | | | ✓ | |
| CmdStartMethodEditing | BL2000\mchavez | 1/5/2022 10:35:10 AM | Start method editing | | | ✓ | |
| CmdImportMethodFromSample | BL2000\mchavez | 1/5/2022 10:35:10 AM | Import method from sample 04JAN15.D | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-------------------------|----------------|----------------------|---|--------|---------|---------|-----------|
| CmdUpdateRetentionTimes | BL2000\mchavez | 1/5/2022 10:35:27 AM | Update retention time for compound 1,4-Dichlorobenzene; 1,3-Dichlorobenzene; 4-Chlorotoluene; 2-Chlorotoluene; 1,2,3-Trichloropropane; Bromobenzene; 1,1,2,2-Tetrachloroethane; p-Bromofluorobenzene; Bromoform; Styrene; o-Xylene; m+p-Xylenes; Ethylbenzene; 1,1,1,2-Tetrachloroethane; Chlorobenzene; 1,2-Dibromoethane; Chlorodibromomethane; 1,3-Dichloropropane; Tetrachloroethene; 1,1,2-Trichloroethane; trans-1,3-Dichloropropene; Toluene; Toluene-d8; cis-1,3-Dichloropropene; Bromodichloromethane; Dibromomethane; 1,2-Dichloropropane; Trichloroethene; 1,2-Dichloroethane; Benzene; 1,2-Dichloroethane-d4; 1,1-Dichloropropene; Carbon tetrachloride; 1,1,1-Trichloroethane; Dibromofluoromethane; Chloroform; Bromochloromethane; Methyl ethyl ketone; cis-1,2-Dichloroethene; 2,2-Dichloropropane; 1,1-Dichloroethane; Methyl tert-butyl ether (MTBE); trans-1,2-Dichloroethene; Methylene chloride; 1,1-Dichloroethene; Trichlorofluoromethane; Chloroethane; Bromomethane; Vinyl chloride; Chloromethane; Dichlorodifluoromethane; 1,4-Dichlorobenzene-d4; Chlorobenzene-d5; Fluorobenzene; 1,2-Dichlorobenzene; | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|--------------------------|----------------|----------------------|--|--------|---------|---------|-----------|
| CmdUpdateQualifierRatios | BL2000\mchavez | 1/5/2022 10:35:32 AM | Update qualifier ratios for compound 1,4-Dichlorobenzene; Update qualifier ratios for compound 1,3-Dichlorobenzene; Update qualifier ratios for compound 4-Chlorotoluene; Update qualifier ratios for compound 2-Chlorotoluene; Update qualifier ratios for compound 1,2,3-Trichloropropane; Update qualifier ratios for compound Bromobenzene; Update qualifier ratios for compound 1,1,2,2-Tetrachloroethane; Update qualifier ratios for compound p-Bromofluorobenzene; Update qualifier ratios for compound Bromoform; Update qualifier ratios for compound Styrene; Update qualifier ratios for compound o-Xylene; Update qualifier ratios for compound m+p-Xylenes; Update qualifier ratios for compound Ethylbenzene; Update qualifier ratios for compound 1,1,1,2-Tetrachloroethane; Update qualifier ratios for compound Chlorobenzene; Update qualifier ratios for compound 1,2-Dibromoethane; Update qualifier ratios for compound Chlorodibromomethane; Update qualifier ratios for compound 1,3-Dichloropropane; Update qualifier ratios for compound Tetrachloroethene; Update qualifier ratios for compound 1,1,2-Trichloroethane; Update qualifier ratios for compound trans-1,3-Dichloropropene; Update qualifier ratios for compound Toluene; Update qualifier ratios for compound Toluene-d8; Update qualifier ratios for compound cis-1,3-Dichloropropene; Update qualifier ratios for compound Bromodichloromethane; Update qualifier ratios for compound Dibromomethane; Update qualifier ratios for compound 1,2-Dichloropropane; Update qualifier ratios for compound Trichloroethene; Update qualifier ratios for compound 1,2-Dichloroethane; Update qualifier ratios for compound Benzene; Update qualifier ratios for compound 1,2-Dichloroethane-d4; Update qualifier ratios for compound 1,1-Dichloropropene; Update qualifier ratios for compound Carbon tetrachloride; Update qualifier ratios for compound 1,1,1-Trichloroethane; Update qualifier ratios for compound Dibromofluoromethane; Update | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|--|--------|---------|---------|-----------|
| | | | qualifier ratios for compound Chloroform; Update qualifier ratios for compound Bromochloromethane; Update qualifier ratios for compound Methyl ethyl ketone; Update qualifier ratios for compound cis-1,2-Dichloroethene; Update qualifier ratios for compound 2,2-Dichloropropane; Update qualifier ratios for compound 1,1-Dichloroethane; Update qualifier ratios for compound Methyl tert-butyl ether (MTBE); Update qualifier ratios for compound trans-1,2-Dichloroethene; Update qualifier ratios for compound Methylene chloride; Update qualifier ratios for compound 1,1-Dichloroethene; Update qualifier ratios for compound Trichlorofluoromethane; Update qualifier ratios for compound Chloroethane; Update qualifier ratios for compound Bromomethane; Update qualifier ratios for compound Vinyl chloride; Update qualifier ratios for compound Chloromethane; Update qualifier ratios for compound Dichlorodifluoromethane; Update qualifier ratios for compound 1,4-Dichlorobenzene-d4; Update qualifier ratios for compound Chlorobenzene-d5; Update qualifier ratios for compound Fluorobenzene; Update qualifier ratios for compound 1,2-Dichlorobenzene; | | | | |
| CmdApplyMethodToAllSamples | BL2000\mchavez | 1/5/2022 10:35:43 AM | Apply method to all samples | | | ✓ | |
| CmdMethodClear | BL2000\mchavez | 1/5/2022 10:35:43 AM | Clear method | | | ✓ | |
| CmdEndMethodEditing | BL2000\mchavez | 1/5/2022 10:35:43 AM | End method editing | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/5/2022 10:36:02 AM | Quantitate all compounds in all samples | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 10:37:04 AM | Manually integrate compound 2-Chlorotoluene in sample 04JAN10.D from x, y = 11.241, 0 to 11.353, 0; result = 1844 | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 10:37:15 AM | Manually integrate compound Bromobenzene in sample 04JAN10.D from x, y = 11.049, 0 to 11.127, 0; result = 2024 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:37:18 AM | Manually integrate qualifier 158.0 of compound Bromobenzene in sample 04JAN10.D from x, y = 11.063, 0 to 11.152, 0; result = 1934 | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|--|--------|---------|---------|-----------|
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 10:37:23 AM | Manually integrate compound 1,1,2,2-Tetrachloroethane in sample 04JAN10.D from x, y = 11.085, 0 to 11.188, 0; result = 1142 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:37:25 AM | Manually integrate qualifier 85.0 of compound 1,1,2,2-Tetrachloroethane in sample 04JAN10.D from x, y = 11.071, 0 to 11.147, 0; result = 834 | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 10:37:35 AM | Manually integrate compound Bromoform in sample 04JAN10.D from x, y = 10.597, 0 to 10.686, 0; result = 708 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:37:36 AM | Manually integrate qualifier 174.5 of compound Bromoform in sample 04JAN10.D from x, y = 10.594, 0 to 10.698, 0; result = 258 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:37:38 AM | Manually integrate qualifier 170.5 of compound Bromoform in sample 04JAN10.D from x, y = 10.603, 0 to 10.672, 0; result = 339 | | | ✓ | |
| CmdSetLevelEnable | BL2000\mchavez | 1/5/2022 10:37:45 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound 1,1,2,2-Tetrachloroethane in sample 04JAN15.D; previous value = True | | | ✓ | |
| CmdSetLevelEnable | BL2000\mchavez | 1/5/2022 10:37:53 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound 2-Chlorotoluene in sample 04JAN15.D; previous value = True | | | ✓ | |
| CmdSetLevelEnable | BL2000\mchavez | 1/5/2022 10:37:55 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound 4-Chlorotoluene in sample 04JAN15.D; previous value = True | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:37:58 AM | Manually integrate qualifier 126.0 of compound 4-Chlorotoluene in sample 04JAN10.D from x, y = 11.367, 0 to 11.467, 0; result = 1839 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:38:03 AM | Manually integrate qualifier 111.0 of compound 1,3-Dichlorobenzene in sample 04JAN10.D from x, y = 12.000, 0 to 12.061, 0; result = 1469 | | | ✓ | |
| CmdSetLevelEnable | BL2000\mchavez | 1/5/2022 10:38:05 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound 1,3-Dichlorobenzene in sample 04JAN15.D; previous value = True | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:38:13 AM | Manually integrate qualifier 111.0 of compound 1,2-Dichlorobenzene in sample 04JAN10.D from x, y = 12.432, 0 to 12.538, 0; result = 1190 | | | ✓ | |
| CmdSetLevelEnable | BL2000\mchavez | 1/5/2022 10:38:15 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound 1,2-Dichlorobenzene in sample 04JAN15.D; previous value = True | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|--|--------|---------|---------|-----------|
| CmdSetLevelEnable | BL2000\mchavez | 1/5/2022 10:38:19 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound 1,4-Dichlorobenzene in sample 04JAN15.D; previous value = True | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:38:25 AM | Manually integrate qualifier 148.0 of compound 1,2-Dichlorobenzene in sample 04JAN10.D from x, y = 12.468, 0 to 12.555, 0; result = 1894 | | | ✓ | |
| CmdSetLevelEnable | BL2000\mchavez | 1/5/2022 10:38:44 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound Styrene in sample 04JAN15.D; previous value = True | | | ✓ | |
| CmdSetLevelEnable | BL2000\mchavez | 1/5/2022 10:38:48 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound o-Xylene in sample 04JAN15.D; previous value = True | | | ✓ | |
| CmdSetLevelEnable | BL2000\mchavez | 1/5/2022 10:38:51 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound m+p-Xylenes in sample 04JAN15.D; previous value = True | | | ✓ | |
| CmdSetLevelEnable | BL2000\mchavez | 1/5/2022 10:38:58 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound Ethylbenzene in sample 04JAN15.D; previous value = True | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:40:02 AM | Manually integrate qualifier 106.0 of compound Ethylbenzene in sample 04JAN10.D, from x, y = 9.883, 0 to 9.953, 0, result = 3266; previous integration is from x, y = 9.914, 0 to 9.953, 0 and previous response = 2097. | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 10:40:07 AM | Manually integrate compound 1,1,1,2-Tetrachloroethane in sample 04JAN10.D from x, y = 9.853, 0 to 9.939, 0; result = 1893 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:40:11 AM | Manually integrate qualifier 133.0 of compound 1,1,1,2-Tetrachloroethane in sample 04JAN10.D from x, y = 9.841, 0 to 9.931, 0; result = 1911 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:40:23 AM | Manually integrate qualifier 114.0 of compound Chlorobenzene in sample 04JAN10.D from x, y = 9.783, 18 to 9.844, 0; result = 1827 | | | ✓ | |
| CmdManuallyIntegrateDropBaseline | BL2000\mchavez | 1/5/2022 10:40:24 AM | Drop baseline for qualifier 114.0 of compound Chlorobenzene in sample 04JAN10.D to y = 0, new integration is from x, y = 9.783, 0 to 9.844, 0 and new response = 1861; previous integration is from x, y = 9.783, 18 to 9.844, 0 and previous response = 1827. | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 10:41:20 AM | Set SampleApproved = True for sample 04JAN10.D; previous value = False | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|---|--------|---------|---------|-----------|
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:41:35 AM | Manually integrate qualifier 64.0 of compound Vinyl chloride in sample 04JAN11.D, from x, y = 1.487, 5730 to 1.520, 4652, result = 5622; previous integration is from x, y = 1.311, 0 to 1.679, 0 and previous response = 180129. | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:41:38 AM | Manually integrate qualifier 64.0 of compound Vinyl chloride in sample 04JAN11.D, from x, y = 1.484, 5832 to 1.520, 4652, result = 5972; previous integration is from x, y = 1.487, 5730 to 1.520, 4652 and previous response = 5622. | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:41:51 AM | Manually integrate qualifier 63.0 of compound 1,1-Dichloroethene in sample 04JAN11.D, from x, y = 2.663, 0 to 2.736, 0, result = 5268; previous integration is from x, y = 2.697, 0 to 2.736, 0 and previous response = 3135. | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 10:41:59 AM | Manually integrate compound trans-1,2-Dichloroethene in sample 04JAN11.D, from x, y = 3.678, 0 to 3.765, 0, result = 9821; previous integration is from x, y = 3.678, 0 to 3.718, 0 and previous response = 5041. | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 10:42:05 AM | Manually integrate compound Methyl tert-butyl ether (MTBE) in sample 04JAN11.D, from x, y = 3.687, 0 to 3.823, 182, result = 11769; previous integration is from x, y = 3.737, 0 to 3.804, 0 and previous response = 10323. | | | ✓ | |
| CmdManuallyIntegrateDropBaseline | BL2000\mchavez | 1/5/2022 10:42:08 AM | Drop baseline for compound Methyl tert-butyl ether (MTBE) in sample 04JAN11.D to y = 0, new integration is from x, y = 3.687, 0 to 3.823, 0 and new response = 12515; previous integration is from x, y = 3.687, 0 to 3.823, 182 and previous response = 11769. | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:42:12 AM | Manually integrate qualifier 57.0 of compound Methyl tert-butyl ether (MTBE) in sample 04JAN11.D, from x, y = 3.681, 0 to 3.821, 0, result = 3045; previous integration is from x, y = 3.709, 0 to 3.776, 0 and previous response = 2643. | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:42:20 AM | Manually integrate qualifier 97.0 of compound 2,2-Dichloropropane in sample 04JAN11.D from x, y = 5.140, 0 to 5.240, 0; result = 3733 | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|---|--------|---------|---------|-----------|
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:42:32 AM | Manually integrate qualifier 191.5 of compound Dibromofluoromethane in sample 04JAN11.D from x, y = 5.809, 0 to 5.918, 0; result = 2020 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:42:45 AM | Manually integrate qualifier 110.0 of compound 1,1-Dichloropropene in sample 04JAN11.D, from x, y = 5.985, 0 to 6.077, 0, result = 5349; previous integration is from x, y = 6.035, 0 to 6.077, 0 and previous response = 3323. | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:42:59 AM | Manually integrate qualifier 98.0 of compound 1,2-Dichloroethane in sample 04JAN11.D from x, y = 6.275, 0 to 6.381, 0; result = 648 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:43:02 AM | Manually integrate qualifier 64.0 of compound 1,2-Dichloroethane in sample 04JAN11.D, from x, y = 6.266, 0 to 6.361, 0, result = 3587; previous integration is from x, y = 6.317, 0 to 6.361, 0 and previous response = 2405. | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:43:11 AM | Manually integrate qualifier 127.0 of compound Bromodichloromethane in sample 04JAN11.D from x, y = 7.549, 0 to 7.627, 0; result = 943 | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 10:43:21 AM | Manually integrate compound 1,1,2-Trichloroethane in sample 04JAN11.D, from x, y = 8.768, 0 to 8.882, 0, result = 5090; previous integration is from x, y = 8.818, 0 to 8.851, 0 and previous response = 2437. | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 10:44:13 AM | Manually integrate compound 1,2,3-Trichloropropane in sample 04JAN11.D from x, y = 11.099, 0 to 11.174, 0; result = 1654 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:44:16 AM | Manually integrate qualifier 112.0 of compound 1,2,3-Trichloropropane in sample 04JAN11.D from x, y = 11.096, 0 to 11.191, 0; result = 1059 | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 10:44:25 AM | Set SampleApproved = True for sample 04JAN11.D; previous value = False | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 10:44:48 AM | Manually integrate compound 1,2,3-Trichloropropane in sample 04JAN12.D, from x, y = 11.099, 0 to 11.180, 0, result = 3200; previous integration is from x, y = 11.141, 0 to 11.180, 0 and previous response = 2198. | | | ✓ | |
| CmdSetLevelEnable | BL2000\mchavez | 1/5/2022 10:45:22 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound Chlorodibromomethane in sample 04JAN15.D; previous value = True | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|------------------------------------|----------------|----------------------|--|--------|---------|---------|-----------|
| CmdSetLevelEnable | BL2000\mchavez | 1/5/2022 10:45:30 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound Tetrachloroethene in sample 04JAN15.D; previous value = True | | | ✓ | |
| CmdSetLevelEnable | BL2000\mchavez | 1/5/2022 10:45:37 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound 1,1,2-Trichloroethane in sample 04JAN15.D; previous value = True | | | ✓ | |
| CmdSetLevelEnable | BL2000\mchavez | 1/5/2022 10:45:40 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound trans-1,3-Dichloropropene in sample 04JAN15.D; previous value = True | | | ✓ | |
| CmdSetLevelEnable | BL2000\mchavez | 1/5/2022 10:45:45 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound Toluene in sample 04JAN15.D; previous value = True | | | ✓ | |
| CmdSetLevelEnable | BL2000\mchavez | 1/5/2022 10:45:57 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound cis-1,3-Dichloropropene in sample 04JAN15.D; previous value = True | | | ✓ | |
| CmdManuallyIntegrate QualifierPeak | BL2000\mchavez | 1/5/2022 10:46:03 AM | Manually integrate qualifier 127.0 of compound Bromodichloromethane in sample 04JAN12.D from x, y = 7.541, 0 to 7.633, 0; result = 2111 | | | ✓ | |
| CmdManuallyIntegrate QualifierPeak | BL2000\mchavez | 1/5/2022 10:46:15 AM | Manually integrate qualifier 98.0 of compound 1,2-Dichloroethane in sample 04JAN12.D from x, y = 6.278, 83 to 6.370, 0; result = 1440 | | | ✓ | |
| CmdManuallyIntegrate DropBaseline | BL2000\mchavez | 1/5/2022 10:46:16 AM | Drop baseline for qualifier 98.0 of compound 1,2-Dichloroethane in sample 04JAN12.D to y = 0, new integration is from x, y = 6.278, 0 to 6.370, 0 and new response = 1669; previous integration is from x, y = 6.278, 83 to 6.370, 0 and previous response = 1440. | | | ✓ | |
| CmdManuallyIntegrate QualifierPeak | BL2000\mchavez | 1/5/2022 10:46:38 AM | Manually integrate qualifier 97.0 of compound 2,2-Dichloropropane in sample 04JAN12.D, from x, y = 5.143, 0 to 5.254, 0, result = 6975; previous integration is from x, y = 5.187, 0 to 5.229, 0 and previous response = 4210. | | | ✓ | |
| CmdManuallyIntegrate QualifierPeak | BL2000\mchavez | 1/5/2022 10:46:55 AM | Manually integrate qualifier 64.0 of compound Vinyl chloride in sample 04JAN12.D, from x, y = 1.473, 6379 to 1.526, 4265, result = 8175; previous integration is from x, y = 1.305, 0 to 1.676, 0 and previous response = 154800. | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|--|--------|---------|---------|-----------|
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:47:03 AM | Manually integrate qualifier 64.0 of compound Vinyl chloride in sample 04JAN12.D, from x, y = 1.467, 4922 to 1.529, 3954, result = 11779; previous integration is from x, y = 1.473, 6379 to 1.526, 4265 and previous response = 8175. | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 10:47:11 AM | Set SampleApproved = True for sample 04JAN12.D; previous value = False | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:47:23 AM | Manually integrate qualifier 64.0 of compound Vinyl chloride in sample 04JAN13.D, from x, y = 1.470, 5496 to 1.517, 5210, result = 15113; previous integration is from x, y = 1.308, 0 to 1.679, 0 and previous response = 148305. | | | ✓ | |
| CmdSetLevelEnable | BL2000\mchavez | 1/5/2022 10:47:46 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound Chloroform in sample 04JAN15.D; previous value = True | | | ✓ | |
| CmdSetLevelEnable | BL2000\mchavez | 1/5/2022 10:47:57 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound 1,1-Dichloropropene in sample 04JAN15.D; previous value = True | | | ✓ | |
| CmdSetLevelEnable | BL2000\mchavez | 1/5/2022 10:48:15 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound Trichloroethene in sample 04JAN15.D; previous value = True | | | ✓ | |
| CmdSetLevelEnable | BL2000\mchavez | 1/5/2022 10:48:21 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound 1,2-Dichloropropane in sample 04JAN15.D; previous value = True | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 10:48:59 AM | Set SampleApproved = True for sample 04JAN13.D; previous value = False | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/5/2022 10:49:20 AM | Quantitate all compounds in all samples | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 10:53:33 AM | Set SampleApproved = True for sample 04JAN17.D; previous value = False | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 10:53:45 AM | Set SampleApproved = True for sample 04JAN19.D; previous value = False | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 10:53:56 AM | Set SampleApproved = True for sample 04JAN21.D; previous value = False | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 10:55:07 AM | Set SampleApproved = True for sample 04JAN23.D; previous value = False | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|--------------|----------------|----------------------|--|--------|---------|---------|-----------|
| CmdCalibrate | BL2000\mchavez | 1/5/2022 10:55:43 AM | Replace level QC with QC sample 04JAN23.D for compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, 1,2-Dichloroethane, Benzene, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1-Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Chloroethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, o-Xylene}; Replace level 8 with Calibration sample 04JAN21.D for compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, 1,2-Dichloroethane, Benzene, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1-Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|------|------|------|--|--------|---------|---------|-----------|
| | | | ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Chloroethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, o-Xylene}; Replace level 7 with Calibration sample 04JAN19.D for compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, 1,2-Dichloroethane, Benzene, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1-Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Chloroethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, o-Xylene}; Replace level 6 with Calibration sample 04JAN17.D for compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, | | | | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|------|------|------|---|--------|---------|---------|-----------|
| | | | Bromodichloromethane, Dibromomethane, 1,2- Dichloropropane, Trichloroethene, 1,2- Dichloroethane, Benzene, 1,2- Dichloroethane-d4, 1,1- Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1- Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2- Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans- 1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Chloroethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, o-Xylene}; Replace level 5 with Calibration sample 04JAN15.D for compounds {1,2- Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3- Trichloropropane, 1,1,2,2- Tetrachloroethane, Bromobenzene, p- Bromofluorobenzene, Bromoform, Styrene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3- Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3- Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2- Dichloropropane, Trichloroethene, 1,2- Dichloroethane, Benzene, 1,2- Dichloroethane-d4, 1,1- Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1- Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2- Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans- 1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Chloroethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, o-Xylene}; Replace level 4 with Calibration sample 04JAN13.D for compounds {1,2- Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3- Trichloropropane, 1,1,2,2- Tetrachloroethane, Bromobenzene, p- | | | | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|------|------|------|--|--------|---------|---------|-----------|
| | | | Bromofluorobenzene, Bromoform, Styrene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, 1,2-Dichloroethane, Benzene, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1-Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Chloroethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, o-Xylene}; Replace level 3 with Calibration sample 04JAN12.D for compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, 1,2-Dichloroethane, Benzene, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1-Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Chloroethane, Bromomethane, Vinyl chloride, | | | | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|------|------|------|--|--------|---------|---------|-----------|
| | | | Chloromethane, Dichlorodifluoromethane, o-Xylene}; Replace level 2 with Calibration sample 04JAN11.D for compounds {1,2- Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3- Trichloropropane, 1,1,2,2- Tetrachloroethane, Bromobenzene, p- Bromofluorobenzene, Bromoform, Styrene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3- Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3- Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2- Dichloropropane, Trichloroethene, 1,2- Dichloroethane, Benzene, 1,2- Dichloroethane-d4, 1,1- Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1- Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2- Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans- 1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Chloroethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, o-Xylene}; Replace level 1 with Calibration sample 04JAN10.D for compounds {1,2- Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3- Trichloropropane, 1,1,2,2- Tetrachloroethane, Bromobenzene, p- Bromofluorobenzene, Bromoform, Styrene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3- Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3- Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2- Dichloropropane, Trichloroethene, 1,2- Dichloroethane, Benzene, 1,2- Dichloroethane-d4, 1,1- Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1- | | | | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-------------------------------------|----------------|----------------------|---|--------|---------|---------|-----------|
| | | | Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Chloroethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, o-Xylene}; | | | | |
| CmdQuantitate | BL2000\mchavez | 1/5/2022 10:55:58 AM | Quantitate all compounds in all samples | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 11:01:11 AM | Manually integrate compound Methylene chloride in sample 04JAN09.D from x, y = 3.296, 0 to 3.383, 0; result = 1661 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 11:01:17 AM | Manually integrate qualifier84.0 of compound Methylene chloride in sample 04JAN09.D from x, y = 3.299, 0 to 3.369, 0; result = 1075 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 11:01:19 AM | Manually integrate qualifier86.0 of compound Methylene chloride in sample 04JAN09.D from x, y = 3.294, 0 to 3.413, 0; result = 694 | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 11:02:10 AM | Manually integrate compound Vinyl chloride in sample 04JAN09.D from x, y = 1.467, 0 to 1.520, 0; result = 73 | | | ✓ | |
| CmdStartMethodEditing | BL2000\mchavez | 1/5/2022 11:02:39 AM | Start method editing | | | ✓ | |
| CmdImportMethodFromSample | BL2000\mchavez | 1/5/2022 11:02:39 AM | Import method from sample 04JAN09.D | | | ✓ | |
| CmdSetMethodTargetCompoundAttribute | BL2000\mchavez | 1/5/2022 11:03:13 AM | Set CurveFit = fitAverageOfResponseFactors for compound Bromomethane; previous value = fitQuadratic | | | ✓ | |
| CmdSetMethodTargetCompoundAttribute | BL2000\mchavez | 1/5/2022 11:03:16 AM | Set CurveFitWeight = weightEqual for compound Bromomethane; previous value = weightOneOverX | | | ✓ | |
| CmdApplyMethodToAllSamples | BL2000\mchavez | 1/5/2022 11:03:28 AM | Apply method to all samples | | | ✓ | |
| CmdMethodClear | BL2000\mchavez | 1/5/2022 11:03:28 AM | Clear method | | | ✓ | |
| CmdEndMethodEditing | BL2000\mchavez | 1/5/2022 11:03:29 AM | End method editing | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/5/2022 11:03:49 AM | Quantitate all compounds in all samples | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 11:05:06 AM | Manually integrate compound Chloroethane in sample 04JAN12.D, from x, y = 1.863, 1400 to 1.922, 1881, result = 14646; previous integration is from x, y = 1.863, 1400 to 1.958, 1400 and previous response = 16843. | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|--------------------------|----------------|----------------------|---|--------|---------|---------|-----------|
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 11:05:19 AM | Manually integrate compound Chloroethane in sample 04JAN11.D, from x, y = 1.869, 1143 to 1.930, 1702, result = 8052; previous integration is from x, y = 1.869, 1143 to 1.941, 1143 and previous response = 9540. | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|--------------|----------------|----------------------|--|--------|---------|---------|-----------|
| CmdCalibrate | BL2000\mchavez | 1/5/2022 11:05:53 AM | Replace level QC with QC sample 04JAN23.D for compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, o-Xylene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, 1,2-Dichloroethane, Benzene, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1-Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, Chloroethane}; Replace level 8 with Calibration sample 04JAN21.D for compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, o-Xylene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, 1,2-Dichloroethane, Benzene, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1- | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|------|------|------|---|--------|---------|---------|-----------|
| | | | Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, Chloroethane}; Replace level 7 with Calibration sample 04JAN19.D for compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, o-Xylene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, 1,2-Dichloroethane, Benzene, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1-Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, Chloroethane}; Replace level 6 with Calibration sample 04JAN17.D for compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, o-Xylene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3- | | | | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|------|------|------|--|--------|---------|---------|-----------|
| | | | Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, 1,2-Dichloroethane, Benzene, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1-Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, Chloroethane}; Replace level 5 with Calibration sample 04JAN15.D for compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, o-Xylene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, 1,2-Dichloroethane, Benzene, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1-Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, Chloroethane}; Replace level 4 with Calibration sample 04JAN13.D for | | | | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|------|------|------|---|--------|---------|---------|-----------|
| | | | compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, o-Xylene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, 1,2-Dichloroethane, Benzene, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1-Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, Chloroethane}; Replace level 3 with Calibration sample 04JAN12.D for compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, o-Xylene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, 1,2-Dichloroethane, Benzene, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1-Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl | | | | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|------|------|------|--|--------|---------|---------|-----------|
| | | | ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, Chloroethane}; Replace level 2 with Calibration sample 04JAN11.D for compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, o-Xylene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, 1,2-Dichloroethane, Benzene, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1-Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, Chloroethane}; Replace level 1 with Calibration sample 04JAN10.D for compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, o-Xylene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3- | | | | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-------------------|----------------|----------------------|---|--------|---------|---------|-----------|
| | | | Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, 1,2-Dichloroethane, Benzene, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1-Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, Chloroethane}; | | | | |
| CmdQuantitate | BL2000\mchavez | 1/5/2022 11:06:12 AM | Quantitate all compounds in all samples | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/5/2022 11:07:28 AM | Quantitate all compounds in all samples | | | ✓ | |
| CmdSaveBatchTable | BL2000\mchavez | 1/5/2022 11:07:47 AM | Save batch D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | | | ✓ | |
| CmdOpenBatchTable | BL2000\mchavez | 1/9/2022 8:45:32 PM | Open batch D:\Org\Data\VOA5975C\VG010422\VG010422_8260B.batch.bin | | | ✓ | |
| CmdSetLevelEnable | BL2000\mchavez | 1/9/2022 8:47:42 PM | Set LevelEnable = True for calibration level 1, levelId = 30 of compound o-Xylene in sample 04JAN09.D; previous value = False | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/9/2022 8:48:01 PM | Quantitate all compounds in all samples | | | ✓ | |
| CmdSetLevelEnable | BL2000\mchavez | 1/9/2022 8:48:47 PM | Set LevelEnable = True for calibration level 1, levelId = 30 of compound m+p-Xylenes in sample 04JAN09.D; previous value = False | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/9/2022 8:49:03 PM | Quantitate all compounds in all samples | | | ✓ | |
| CmdSetLevelEnable | BL2000\mchavez | 1/9/2022 8:49:35 PM | Set LevelEnable = True for calibration level 1, levelId = 30 of compound Ethylbenzene in sample 04JAN09.D; previous value = False | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/9/2022 8:49:50 PM | Quantitate all compounds in all samples | | | ✓ | |
| CmdSetLevelEnable | BL2000\mchavez | 1/9/2022 8:50:18 PM | Set LevelEnable = True for calibration level 1, levelId = 30 of compound Styrene in sample 04JAN09.D; previous value = False | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-------------------|----------------|---------------------|--|--------|---------|---------|-----------|
| CmdQuantitate | BL2000\mchavez | 1/9/2022 8:50:35 PM | Quantitate all compounds in all samples | | | ✓ | |
| CmdSetLevelEnable | BL2000\mchavez | 1/9/2022 8:50:51 PM | Set LevelEnable = True for calibration level 1, levelId = 30 of compound Tetrachloroethene in sample 04JAN09.D; previous value = False | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/9/2022 8:51:06 PM | Quantitate all compounds in all samples | | | ✓ | |
| CmdSetLevelEnable | BL2000\mchavez | 1/9/2022 8:51:27 PM | Set LevelEnable = True for calibration level 1, levelId = 30 of compound Toluene in sample 04JAN09.D; previous value = False | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/9/2022 8:51:42 PM | Quantitate all compounds in all samples | | | ✓ | |
| CmdSetLevelEnable | BL2000\mchavez | 1/9/2022 8:52:26 PM | Set LevelEnable = True for calibration level 1, levelId = 30 of compound trans-1,3-Dichloropropene in sample 04JAN09.D; previous value = False | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/9/2022 8:52:42 PM | Quantitate all compounds in all samples | | | ✓ | |
| CmdSetLevelEnable | BL2000\mchavez | 1/9/2022 8:52:55 PM | Set LevelEnable = False for calibration level 1, levelId = 30 of compound trans-1,3-Dichloropropene in sample 04JAN09.D; previous value = True | | | ✓ | |
| CmdSetLevelEnable | BL2000\mchavez | 1/9/2022 8:53:25 PM | Set LevelEnable = True for calibration level 1, levelId = 30 of compound Benzene in sample 04JAN09.D; previous value = False | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/9/2022 8:53:41 PM | Quantitate all compounds in all samples | | | ✓ | |
| CmdSetLevelEnable | BL2000\mchavez | 1/9/2022 8:54:07 PM | Set LevelEnable = True for calibration level 1, levelId = 30 of compound Chloroform in sample 04JAN09.D; previous value = False | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/9/2022 8:54:23 PM | Quantitate all compounds in all samples | | | ✓ | |
| CmdSetLevelEnable | BL2000\mchavez | 1/9/2022 8:54:39 PM | Set LevelEnable = True for calibration level 1, levelId = 30 of compound 1,3-Dichlorobenzene in sample 04JAN09.D; previous value = False | | | ✓ | |
| CmdSetLevelEnable | BL2000\mchavez | 1/9/2022 8:54:49 PM | Set LevelEnable = True for calibration level 1, levelId = 30 of compound 1,4-Dichlorobenzene in sample 04JAN09.D; previous value = False | | | ✓ | |
| CmdSetLevelEnable | BL2000\mchavez | 1/9/2022 8:54:54 PM | Set LevelEnable = True for calibration level 1, levelId = 30 of compound 1,2-Dichlorobenzene in sample 04JAN09.D; previous value = False | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/9/2022 8:55:10 PM | Quantitate all compounds in all samples | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|------------------------------|----------------|---------------------|---|--------|---------|---------|-----------|
| CmdSetLevelEnable | BL2000\mchavez | 1/9/2022 8:56:06 PM | Set LevelEnable = True for calibration level 1, levelId = 30 of compound 1,2-Dichloroethane in sample 04JAN09.D; previous value = False | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/9/2022 8:56:22 PM | Quantitate all compounds in all samples | | | ✓ | |
| CmdImportSamplesFromWorklist | BL2000\mchavez | 1/9/2022 8:56:50 PM | Add samples from worklist: D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/9/2022 8:57:23 PM | Set SampleType = Calibration for sample 04JAN15CC.D; previous value = Sample | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/9/2022 8:57:29 PM | Set LevelName = 5 for sample 04JAN15CC.D; previous value = | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/9/2022 8:57:56 PM | Quantitate all compounds in all samples | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/9/2022 8:58:36 PM | Set SampleType = CC for sample 04JAN15CC.D; previous value = Calibration | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/9/2022 8:58:43 PM | Set LevelName = CC for sample 04JAN15CC.D; previous value = 5 | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/9/2022 8:59:05 PM | Set UserDefined = Reimported midpoint as CC for sample 04JAN15CC.D; previous value = | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/9/2022 8:59:31 PM | Set SampleName = CC010422 for sample 04JAN15CC.D; previous value = ICAL010422_5 | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|----------------------------|----------------|---------------------|---|--------|---------|---------|-----------|
| CmdCalibrate | BL2000\mchavez | 1/9/2022 8:59:53 PM | Replace level CC with CC sample 04JAN15CC.D for compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, o-Xylene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, Benzene, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1-Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Chloroethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, 1,2-Dichloroethane}; | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/9/2022 9:00:09 PM | Quantitate all compounds in all samples | | | ✓ | |
| CmdStartMethodEditing | BL2000\mchavez | 1/9/2022 9:00:22 PM | Start method editing | | | ✓ | |
| CmdImportMethodFrom Sample | BL2000\mchavez | 1/9/2022 9:00:22 PM | Import method from sample 04JAN23.D | | | ✓ | |
| CmdSaveMethodAs | BL2000\mchavez | 1/9/2022 9:00:57 PM | Save method to file \\MASSHUNTER\Org\Data\Methods\Quant\VOA5975C\VOA5975C_010422_CAL.m | | | ✓ | |
| CmdSaveMethodAs | BL2000\mchavez | 1/9/2022 9:02:42 PM | Save method to file \\MASSHUNTER\Org\Data\Methods\Quant\VOA5975C\VOA5975C_010422_CAL\VOA5975C_8260B_SHT_DoD_L4_010422.m | | | ✓ | |
| CmdMethodClear | BL2000\mchavez | 1/9/2022 9:02:55 PM | Clear method | | | ✓ | |
| CmdEndMethodEditing | BL2000\mchavez | 1/9/2022 9:02:56 PM | End method editing | | | ✓ | |
| CmdStartMethodEditing | BL2000\mchavez | 1/9/2022 9:03:07 PM | Start method editing | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|---|--------|---------|---------|-----------|
| CmdImportMethodFromFile | BL2000\mchavez | 1/9/2022 9:03:07 PM | Import method from file \\MASSHUNTER\Org\Data\Methods\Quant\VOA5975C\VOA5975C_010422_CAL\VOA5975C_8260B_SHT_DoD_L4_010422.m | | | ✓ | |
| CmdApplyMethodToAllSamples | BL2000\mchavez | 1/9/2022 9:03:19 PM | Apply method to all samples | | | ✓ | |
| CmdMethodClear | BL2000\mchavez | 1/9/2022 9:03:19 PM | Clear method | | | ✓ | |
| CmdEndMethodEditing | BL2000\mchavez | 1/9/2022 9:03:20 PM | End method editing | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/9/2022 9:03:36 PM | Quantitate all compounds in all samples | | | ✓ | |
| CmdSaveBatchTable | BL2000\mchavez | 1/9/2022 9:04:21 PM | Save batch D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | | | ✓ | |
| CmdOpenBatchTable | BL2000\mchavez | 1/10/2022 2:13:24 PM | Open batch D:\Org\Data\VOA5975C\VG010422\VG010422_8260B.batch.bin | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 2:13:38 PM | Set SampleApproved = True for sample 04JAN08.D; previous value = False | | | ✓ | |
| CmdZeroOutPeak | BL2000\mchavez | 1/10/2022 2:14:50 PM | Zero out primary peak of compound Chloromethane in sample 04JAN09.D | | | ✓ | |
| CmdZeroOutPeak | BL2000\mchavez | 1/10/2022 2:14:56 PM | Zero out primary peak of compound Vinyl chloride in sample 04JAN09.D | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 2:15:19 PM | Manually integrate compound Benzene in sample 04JAN09.D from x, y = 6.250, 0 to 6.311, 0; result = 381 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 2:15:21 PM | Manually integrate qualifier 77.0 of compound Benzene in sample 04JAN09.D from x, y = 6.258, 0 to 6.308, 0; result = 86 | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 2:16:46 PM | Set SampleApproved = True for sample 04JAN09.D; previous value = False | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 2:17:02 PM | Set UserAnnotation = NI for compound Methylene chloride in sample 04JAN09.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 2:17:09 PM | Set UserAnnotation = NI for compound Benzene in sample 04JAN09.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 2:18:45 PM | Set UserAnnotation = NI for compound Tetrachloroethene in sample 04JAN10.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 2:18:48 PM | Set UserAnnotation = NI for compound Chlorodibromomethane in sample 04JAN10.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 2:18:53 PM | Set UserAnnotation = NI for compound 1,2-Dibromoethane in sample 04JAN10.D; previous value = | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|---|--------|---------|---------|-----------|
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 2:18:58 PM | Set UserAnnotation = NI for compound 1,1,1,2-Tetrachloroethane in sample 04JAN10.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 2:19:02 PM | Set UserAnnotation = NI for compound Bromoform in sample 04JAN10.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 2:19:08 PM | Set UserAnnotation = NI for compound 1,1,2,2-Tetrachloroethane in sample 04JAN10.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 2:19:13 PM | Set UserAnnotation = NI for compound Bromobenzene in sample 04JAN10.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 2:19:30 PM | Set UserAnnotation = NI for compound 2-Chlorotoluene in sample 04JAN10.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 2:20:15 PM | Set UserAnnotation = GT for compound Chloroethane in sample 04JAN11.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 2:20:34 PM | Set UserAnnotation = LT for compound trans-1,2-Dichloroethene in sample 04JAN11.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 2:25:39 PM | Set UserAnnotation = LT for compound Methyl tert-butyl ether (MTBE) in sample 04JAN11.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 2:26:14 PM | Set UserAnnotation = LT for compound 1,1,2-Trichloroethane in sample 04JAN11.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 2:26:26 PM | Set UserAnnotation = NI for compound 1,2,3-Trichloropropane in sample 04JAN11.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 2:26:46 PM | Set UserAnnotation = LT for compound 1,2,3-Trichloropropane in sample 04JAN12.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 2:26:59 PM | Set UserAnnotation = GT for compound Chloroethane in sample 04JAN12.D; previous value = | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 3:00:42 PM | Manually integrate qualifier 148.0 of compound 1,4-Dichlorobenzene in sample 04JAN10.D, from x, y = 12.109, 0 to 12.145, 0, result = 2520; previous integration is from x, y = 12.084, 0 to 12.145, 0 and previous response = 3603. | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 3:00:52 PM | Manually integrate qualifier 111.0 of compound 1,4-Dichlorobenzene in sample 04JAN10.D, from x, y = 12.123, 0 to 12.148, 0, result = 1067; previous integration is from x, y = 12.075, 0 to 12.123, 0 and previous response = 3515. | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|---|--------|---------|---------|-----------|
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 3:01:20 PM | Manually integrate qualifier 91.0 of compound o-Xylene in sample 04JAN10.D, from x, y = 10.405, 0 to 10.483, 0, result = 6062; previous integration is from x, y = 10.405, 0 to 10.466, 0 and previous response = 6034. | | | ✓ | |
| CmdClearManualIntegration | BL2000\mchavez | 1/10/2022 3:01:29 PM | Clear manual integration of qualifier 91.0 for compound o-Xylene in sample 04JAN10.D | | | ✓ | |
| CmdSetLevelEnable | BL2000\mchavez | 1/10/2022 3:07:00 PM | Set LevelEnable = False for calibration level 1, levelId = 30 of compound o-Xylene in sample 04JAN23.D; previous value = True | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/10/2022 3:07:39 PM | Quantitate all compounds in all samples | | | ✓ | |
| CmdSaveBatchTable | BL2000\mchavez | 1/10/2022 3:12:09 PM | Save batch D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | | | ✓ | |
| CmdOpenBatchTable | BL2000\mchavez | 1/11/2022 8:47:03 AM | Open batch D:\Org\Data\VOA5975C\VG010422\VG010422_8260B.batch.bin | | | ✓ | |
| CmdStartMethodEditing | BL2000\mchavez | 1/11/2022 8:47:16 AM | Start method editing | | | ✓ | |
| CmdImportMethodFromSample | BL2000\mchavez | 1/11/2022 8:47:16 AM | Import method from sample 04JAN01.D | | | ✓ | |
| CmdSaveMethodAs | BL2000\mchavez | 1/11/2022 8:47:26 AM | Save method to file \\MASSHUNTER\Org\Data\Methods\Quant\VOA5975C\VOA5975C_010422_CAL\VOA5975C_8260B_SHT_DoD_L4_010422.m | | | ✓ | |
| CmdApplyMethodToAllSamples | BL2000\mchavez | 1/11/2022 8:48:57 AM | Apply method to all samples | | | ✓ | |
| CmdMethodClear | BL2000\mchavez | 1/11/2022 8:48:57 AM | Clear method | | | ✓ | |
| CmdEndMethodEditing | BL2000\mchavez | 1/11/2022 8:48:58 AM | End method editing | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/11/2022 8:49:22 AM | Quantitate all compounds in all samples | | | ✓ | |
| CmdSaveBatchTable | BL2000\mchavez | 1/11/2022 8:54:59 AM | Save batch D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | | | ✓ | |
| CmdOpenBatchTable | BL2000\mchavez | 2/28/2022 1:48:49 PM | Open batch D:\Org\Data\VOA5975C\VG010422\VG010422_8260B.batch.bin | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 2/28/2022 1:49:23 PM | Set UserAnnotation = NI for compound Bromomethane in sample 04JAN10.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 2/28/2022 1:49:29 PM | Set UserAnnotation = GT for compound Chloroethane in sample 04JAN10.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 2/28/2022 1:49:34 PM | Set UserAnnotation = NI for compound 1,1-Dichloroethene in sample 04JAN10.D; previous value = | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-------------------------------|----------------|----------------------|---|--------|---------|---------|-----------|
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 2/28/2022 1:49:38 PM | Set UserAnnotation = NI for compound trans-1,2-Dichloroethene in sample 04JAN10.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 2/28/2022 1:49:43 PM | Set UserAnnotation = NI for compound Methyl tert-butyl ether (MTBE) in sample 04JAN10.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 2/28/2022 1:49:46 PM | Set UserAnnotation = NI for compound 2,2-Dichloropropane in sample 04JAN10.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 2/28/2022 1:49:51 PM | Set UserAnnotation = NI for compound cis-1,2-Dichloroethene in sample 04JAN10.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 2/28/2022 1:49:55 PM | Set UserAnnotation = NI for compound Bromochloromethane in sample 04JAN10.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 2/28/2022 1:49:59 PM | Set UserAnnotation = NI for compound Dibromofluoromethane in sample 04JAN10.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 2/28/2022 1:50:03 PM | Set UserAnnotation = NI for compound 1,2-Dichloroethane-d4 in sample 04JAN10.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 2/28/2022 1:50:06 PM | Set UserAnnotation = NI for compound 1,2-Dichloroethane in sample 04JAN10.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 2/28/2022 1:50:10 PM | Set UserAnnotation = NI for compound Trichloroethene in sample 04JAN10.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 2/28/2022 1:50:14 PM | Set UserAnnotation = NI for compound Dibromomethane in sample 04JAN10.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 2/28/2022 1:50:19 PM | Set UserAnnotation = NI for compound trans-1,3-Dichloropropene in sample 04JAN10.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 2/28/2022 1:50:23 PM | Set UserAnnotation = NI for compound 1,1,2-Trichloroethane in sample 04JAN10.D; previous value = | | | ✓ | |
| CmdSaveBatchTable | BL2000\mchavez | 2/28/2022 1:54:50 PM | Save batch D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | | | ✓ | |
| GenerateReport | BL2000\mchavez | 2/28/2022 1:56:23 PM | Generates report - Method: \\MASSHUNTER\Org\reports\LevelIV_Reports\Calibration\01_Init_Cal+Gen_Calibration+Gen_ResultsSummary.m, Output Path: D:\Org\Data\VOA5975C\VG010422\QuantReports\VG010422_8260B | | | ✓ | |
| CmdStartMethodEditing | BL2000\mchavez | 2/28/2022 1:57:20 PM | Start method editing | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|----------------------------|----------------|----------------------|---|--------|---------|---------|-----------|
| CmdImportMethodFromFile | BL2000\mchavez | 2/28/2022 1:57:21 PM | Import method from file \\MASSHUNTER\Org\Data\Methods\Quant\VOA5975C\VOA5975C_010422_CAL\VOA5975C_8260B_SHT_DoD_L4_010422.m | | | ✓ | |
| CmdApplyMethodToAllSamples | BL2000\mchavez | 2/28/2022 1:57:33 PM | Apply method to all samples | | | ✓ | |
| CmdMethodClear | BL2000\mchavez | 2/28/2022 1:57:33 PM | Clear method | | | ✓ | |
| CmdEndMethodEditing | BL2000\mchavez | 2/28/2022 1:57:33 PM | End method editing | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 2/28/2022 1:57:54 PM | Quantitate all compounds in all samples | | | ✓ | |
| CmdSaveBatchTable | BL2000\mchavez | 2/28/2022 1:59:46 PM | Save batch D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | | | ✓ | |
| GenerateReport | BL2000\mchavez | 2/28/2022 2:00:55 PM | Generates report - Method: \\MASSHUNTER\Org\reports\LevelIV_Reports\Calibration\01_Init_Cal+Gen_Calibration+Gen_ResultsSummary.m, Output Path: D:\Org\Data\VOA5975C\VG010422\QuantReports\VG010422_8260B-1 | | | ✓ | |

Energy Laboratories Inc

ANALYTICAL RUN Summary

28-Feb-22

Run ID VOA5975C.I_220105A

| |
|---------------------------------|
| Run Start Date: 1/5/2022 |
| Analyst: Melissa Chavez |
| Ical: |
| Column ID: |
| Comments: |

| Std ID | Std Name | Std Amount | Std Units | Samp Amount | Samp Units | SampType | Expiration Date |
|-----------|---|------------|-----------|-------------|------------|------------|-----------------|
| VOCF3517 | Internal Standard / Surrogates (INT/SURR) | 8.4 | ul | 42 | ml | ALL (TUNE | 12/31/2022 |
| VOCF3529B | 2nd Source MtBE | 1.05 | ul | 42 | ml | LCS, MS, M | 1/29/2022 |
| VOCF3546A | Liquids | 1.05 | ul | 42 | ml | CCV | 1/13/2022 |
| VOCF3549 | 2nd Source Ketones | 1.05 | ul | 42 | ml | LCS, MS, M | 1/15/2022 |
| VOCF3550 | Ketones | 1.05 | ul | 42 | ml | CCV | 1/16/2022 |
| VOCF3558B | 2nd Source Liquids | 1.05 | ul | 42 | ml | LCS, MS, M | 2/27/2022 |
| VOCF3559A | MtBE | 1.05 | ul | 42 | ml | CCV | 1/27/2022 |
| VOCF3562A | Gases | 1.05 | ul | 42 | ml | CCV | 1/10/2022 |
| VOCF3566A | 2nd Source Gases | 1.05 | ul | 42 | ml | LCS, MS, M | 1/11/2022 |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|--------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|-------|------|---|
| 14971523 | 05JAN02_D_TU | VOC-8260-BFB | TUNE | DA5975C\VG010 | 1/5/2022 9:49:00 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 173, % of mass 174 | A | % | 1.6 | 1.6 | | 100 | 0 | 0 | 0 | 0 | 0 | 2% | 0 | 2 | 0% | |
| 174, % of mass 95 | A | % | 92 | 92 | | 100 | 0 | 0 | 0 | 0 | 0 | 92% | 50 | 99.99 | 0% | |
| 175, % of mass 174 | A | % | 7.2 | 7.2 | | 100 | 0 | 0 | 0 | 0 | 0 | 7% | 5 | 9 | 0% | |
| 176, % of mass 174 | A | % | 96.9 | 96.9 | | 100 | 0 | 0 | 0 | 0 | 0 | 97% | 95 | 101 | 0% | |
| 177, % of mass 176 | A | % | 7.1 | 7.1 | | 100 | 0 | 0 | 0 | 0 | 0 | 7% | 5 | 9 | 0% | |
| 50, % of mass 95 | A | % | 20.8 | 20.8 | | 100 | 0 | 0 | 0 | 0 | 0 | 21% | 15 | 40 | 0% | |
| 75, % of mass 95 | A | % | 48.4 | 48.4 | | 100 | 0 | 0 | 0 | 0 | 0 | 48% | 30 | 60 | 0% | |
| 95, Base Peak | A | % | 100 | 100 | | 100 | 0 | 0 | 0 | 0 | 0 | 100% | 0 | 100 | 0% | |
| 96, % of mass 95 | A | % | 6.4 | 6.4 | | 100 | 0 | 0 | 0 | 0 | 0 | 6% | 5 | 9 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971524 | CCV010522_ | VOC-8260-W-Q | CCV | DA5975CVVG010:1/5/2022 | 10:28:4 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A | ug/L | 133.50715 | 5.340286 | | 5 | 0 | 0 | 0.101 | 0.5 | 500 | 107% | 80 | 120 | 0% | |
| 1,1,1-Trichloroethane | A | ug/L | 129.2681 | 5.170724 | | 5 | 0 | 0 | 0.131 | 0.5 | 500 | 103% | 80 | 120 | 0% | |
| 1,1,2,2-Tetrachloroethane | A | ug/L | 140.25396 | 5.6101584 | | 5 | 0 | 0 | 0.0872 | 0.5 | 500 | 112% | 80 | 120 | 0% | |
| 1,1,2-Trichloroethane | A | ug/L | 139.08201 | 5.5632804 | | 5 | 0 | 0 | 0.108 | 0.5 | 500 | 111% | 80 | 120 | 0% | |
| 1,1-Dichloroethane | A | ug/L | 137.31142 | 5.4924568 | | 5 | 0 | 0 | 0.135 | 0.5 | 500 | 110% | 80 | 120 | 0% | |
| 1,1-Dichloroethene | A | ug/L | 129.17613 | 5.1670452 | | 5 | 0 | 0 | 0.141 | 0.5 | 500 | 103% | 80 | 120 | 0% | |
| 1,1-Dichloropropene | A | ug/L | 130.63845 | 5.225538 | | 5 | 0 | 0 | 0.083 | 0.5 | 500 | 105% | 80 | 120 | 0% | |
| 1,2,3-Trichloropropane | A | ug/L | 141.95667 | 5.6782668 | | 5 | 0 | 0 | 0.235 | 0.5 | 500 | 114% | 80 | 120 | 0% | |
| 1,2-Dibromoethane | A | ug/L | 136.93185 | 5.477274 | | 5 | 0 | 0 | 0.0916 | 0.5 | 500 | 110% | 80 | 120 | 0% | |
| 1,2-Dichlorobenzene | A | ug/L | 128.75548 | 5.1502192 | | 5 | 0 | 0 | 0.0746 | 0.5 | 500 | 103% | 80 | 120 | 0% | |
| 1,2-Dichloroethane | A | ug/L | 135.03684 | 5.4014736 | | 5 | 0 | 0 | 0.116 | 0.5 | 500 | 108% | 80 | 120 | 0% | |
| 1,2-Dichloropropane | A | ug/L | 136.29508 | 5.4518032 | | 5 | 0 | 0 | 0.0847 | 0.5 | 500 | 109% | 80 | 120 | 0% | |
| 1,3-Dichlorobenzene | A | ug/L | 129.89302 | 5.1957208 | | 5 | 0 | 0 | 0.0803 | 0.5 | 500 | 104% | 80 | 120 | 0% | |
| 1,3-Dichloropropane | A | ug/L | 140.48351 | 5.6193404 | | 5 | 0 | 0 | 0.0791 | 0.5 | 500 | 112% | 80 | 120 | 0% | |
| 1,4-Dichlorobenzene | A | ug/L | 131.37325 | 5.25493 | | 5 | 0 | 0 | 0.0858 | 0.5 | 500 | 105% | 80 | 120 | 0% | |
| 2,2-Dichloropropane | A | ug/L | 133.6522 | 5.346088 | | 5 | 0 | 0 | 0.186 | 0.5 | 500 | 107% | 80 | 120 | 0% | |
| 2-Chlorotoluene | A | ug/L | 132.18454 | 5.2873816 | | 5 | 0 | 0 | 0.0876 | 0.5 | 500 | 106% | 80 | 120 | 0% | |
| 4-Chlorotoluene | A | ug/L | 136.46816 | 5.4587264 | | 5 | 0 | 0 | 0.0728 | 0.5 | 500 | 109% | 80 | 120 | 0% | |
| Benzene | A | ug/L | 135.33085 | 5.413234 | | 5 | 0 | 0 | 0.0914 | 0.5 | 500 | 108% | 80 | 120 | 0% | |
| Bromobenzene | A | ug/L | 134.77223 | 5.3908892 | | 5 | 0 | 0 | 0.0831 | 0.5 | 500 | 108% | 80 | 120 | 0% | |
| Bromochloromethane | A | ug/L | 140.79267 | 5.6317068 | | 5 | 0 | 0 | 0.141 | 0.5 | 500 | 113% | 80 | 120 | 0% | |
| Bromodichloromethane | A | ug/L | 134.29565 | 5.371826 | | 5 | 0 | 0 | 0.12 | 0.5 | 500 | 107% | 80 | 120 | 0% | |
| Bromoform | A | ug/L | 140.26683 | 5.6106732 | | 5 | 0 | 0 | 0.119 | 0.5 | 500 | 112% | 80 | 120 | 0% | |
| Bromomethane | A | ug/L | 130.74018 | 5.2296072 | | 5 | 0 | 0 | 0.253 | 0.5 | 500 | 105% | 80 | 120 | 0% | |
| Carbon tetrachloride | A | ug/L | 128.23107 | 5.1292428 | | 5 | 0 | 0 | 0.143 | 0.5 | 500 | 103% | 80 | 120 | 0% | |
| Chlorobenzene | A | ug/L | 132.67301 | 5.3069204 | | 5 | 0 | 0 | 0.0914 | 0.5 | 500 | 106% | 80 | 120 | 0% | |
| Chlorodibromomethane | A | ug/L | 139.12487 | 5.5649948 | | 5 | 0 | 0 | 0.0841 | 0.5 | 500 | 111% | 80 | 120 | 0% | |
| Chloroethane | A | ug/L | 121.24857 | 4.8499428 | | 5 | 0 | 0 | 0.169 | 0.5 | 500 | 97% | 80 | 120 | 0% | |
| Chloroform | A | ug/L | 128.66267 | 5.1465068 | | 5 | 0 | 0 | 0.0789 | 0.5 | 500 | 103% | 80 | 120 | 0% | |
| Chloromethane | A | ug/L | 121.36946 | 4.8547784 | | 5 | 0 | 0 | 0.162 | 0.5 | 500 | 97% | 80 | 120 | 0% | |
| cis-1,2-Dichloroethene | A | ug/L | 137.38746 | 5.4954984 | | 5 | 0 | 0 | 0.108 | 0.5 | 500 | 110% | 80 | 120 | 0% | |
| cis-1,3-Dichloropropene | A | ug/L | 131.91959 | 5.2767836 | | 5 | 0 | 0 | 0.073 | 0.5 | 500 | 106% | 80 | 120 | 0% | |
| Dibromomethane | A | ug/L | 136.15206 | 5.4460824 | | 5 | 0 | 0 | 0.147 | 0.5 | 500 | 109% | 80 | 120 | 0% | |
| Dichlorodifluoromethane | A | ug/L | 121.63771 | 4.8655084 | | 5 | 0 | 0 | 0.175 | 0.5 | 500 | 97% | 80 | 120 | 0% | |
| Ethylbenzene | A | ug/L | 132.4334 | 5.297336 | | 5 | 0 | 0 | 0.0836 | 0.5 | 500 | 106% | 80 | 120 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|--------------------------------|------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971524 | CCV010522_ | VOC-8260-W-Q | CCV | DA5975C\VG010:1/5/2022 | 10:28:4 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| m+p-Xylenes | A | ug/L | 268.36958 | 10.7347832 | | 10 | 0 | 0 | 0.15 | 0.5 | 1000 | 107% | 80 | 120 | 0% | |
| Methyl ethyl ketone | A | ug/L | 1283.79984 | 51.3519936 | | 50 | 0 | 0 | 1.77 | 10 | 5000 | 103% | 80 | 120 | 0% | |
| Methyl tert-butyl ether (MTBE) | A | ug/L | 129.87058 | 5.1948232 | | 5 | 0 | 0 | 0.101 | 0.5 | 500 | 104% | 80 | 120 | 0% | |
| Methylene chloride | A | ug/L | 126.69785 | 5.067914 | | 5 | 0 | 0 | 0.338 | 0.5 | 500 | 101% | 80 | 120 | 0% | |
| o-Xylene | A | ug/L | 133.90371 | 5.3561484 | | 5 | 0 | 0 | 0.0604 | 0.5 | 500 | 107% | 80 | 120 | 0% | |
| Styrene | A | ug/L | 140.5011 | 5.620044 | | 5 | 0 | 0 | 0.067 | 0.5 | 500 | 112% | 80 | 120 | 0% | |
| Tetrachloroethene | A | ug/L | 129.30964 | 5.1723856 | | 5 | 0 | 0 | 0.0671 | 0.5 | 500 | 103% | 80 | 120 | 0% | |
| Toluene | A | ug/L | 136.47421 | 5.4589684 | | 5 | 0 | 0 | 0.0679 | 0.5 | 500 | 109% | 80 | 120 | 0% | |
| trans-1,2-Dichloroethene | A | ug/L | 132.27222 | 5.2908888 | | 5 | 0 | 0 | 0.125 | 0.5 | 500 | 106% | 80 | 120 | 0% | |
| trans-1,3-Dichloropropene | A | ug/L | 145.66628 | 5.8266512 | | 5 | 0 | 0 | 0.0846 | 0.5 | 500 | 117% | 80 | 120 | 0% | |
| Trichloroethene | A | ug/L | 131.52849 | 5.2611396 | | 5 | 0 | 0 | 0.0993 | 0.5 | 500 | 105% | 80 | 120 | 0% | |
| Trichlorofluoromethane | A | ug/L | 124.38242 | 4.9752968 | | 5 | 0 | 0 | 0.134 | 0.5 | 500 | 100% | 80 | 120 | 0% | |
| Vinyl chloride | A | ug/L | 124.08337 | 4.9633348 | | 5 | 0 | 0 | 0.153 | 0.5 | 500 | 99% | 80 | 120 | 0% | |
| 1,4-Dichlorobenzene-d4 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 0 | 0 | 0% | |
| Chlorobenzene-d5 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 0 | 0 | 0% | |
| Fluorobenzene | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 0 | 0 | 0% | |
| Xylenes, Total | M | ug/L | 402.27329 | 16.0909316 | | 15 | 0 | 0 | 0.0604 | 0.5 | 1500 | 107% | 80 | 120 | 0% | |
| 1,2-Dichloroethane-d4 | S | ug/L | 290.732 | 11.62928 | | 10 | 0 | 0 | 0.229 | 0.5 | 500 | 116% | 80 | 120 | 0% | |
| Dibromofluoromethane | S | ug/L | 281.66353 | 11.2665412 | | 10 | 0 | 0 | 0.129 | 0.5 | 500 | 113% | 80 | 120 | 0% | |
| p-Bromofluorobenzene | S | ug/L | 266.74216 | 10.6696864 | | 10 | 0 | 0 | 0.149 | 0.5 | 500 | 107% | 80 | 120 | 0% | |
| Toluene-d8 | S | ug/L | 277.8286 | 11.113144 | | 10 | 0 | 0 | 0.23 | 0.5 | 500 | 111% | 80 | 120 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971525 | LCS010522_ | VOC-8260-W-Q | LCS-DOD | DA5975C\VG010:1/5/2022 | 11:27:3 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A | ug/L | 127.23054 | 5.0892216 | | 5 | 0 | 0 | 0.101 | 0.5 | 500 | 102% | 78 | 124 | 0% | |
| 1,1,1-Trichloroethane | A | ug/L | 126.12815 | 5.045126 | | 5 | 0 | 0 | 0.131 | 0.5 | 500 | 101% | 74 | 131 | 0% | |
| 1,1,2,2-Tetrachloroethane | A | ug/L | 133.32389 | 5.3329556 | | 5 | 0 | 0 | 0.0872 | 0.5 | 500 | 107% | 71 | 121 | 0% | |
| 1,1,2-Trichloroethane | A | ug/L | 132.3073 | 5.292292 | | 5 | 0 | 0 | 0.108 | 0.5 | 500 | 106% | 80 | 119 | 0% | |
| 1,1-Dichloroethane | A | ug/L | 139.1372 | 5.565488 | | 5 | 0 | 0 | 0.135 | 0.5 | 500 | 111% | 77 | 125 | 0% | |
| 1,1-Dichloroethene | A | ug/L | 136.91271 | 5.4765084 | | 5 | 0 | 0 | 0.141 | 0.5 | 500 | 110% | 71 | 131 | 0% | |
| 1,1-Dichloropropene | A | ug/L | 122.64472 | 4.9057888 | | 5 | 0 | 0 | 0.083 | 0.5 | 500 | 98% | 79 | 125 | 0% | |
| 1,2,3-Trichloropropane | A | ug/L | 131.68394 | 5.2673576 | | 5 | 0 | 0 | 0.235 | 0.5 | 500 | 105% | 73 | 125 | 0% | |
| 1,2-Dibromoethane | A | ug/L | 133.82951 | 5.3531804 | | 5 | 0 | 0 | 0.0916 | 0.5 | 500 | 107% | 78 | 122 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|--------------------------------|------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971525 | LCS010522_ | VOC-8260-W-Q | LCS-DOD | DA5975C\VG010:1/5/2022 | 11:27:3 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,2-Dichlorobenzene | A | ug/L | 131.99403 | 5.2797612 | | 5 | 0 | 0 | 0.0746 | 0.5 | 500 | 106% | 80 | 119 | 0% | |
| 1,2-Dichloroethane | A | ug/L | 127.24721 | 5.0898884 | | 5 | 0 | 0 | 0.116 | 0.5 | 500 | 102% | 73 | 128 | 0% | |
| 1,2-Dichloropropane | A | ug/L | 128.20824 | 5.1283296 | | 5 | 0 | 0 | 0.0847 | 0.5 | 500 | 103% | 78 | 122 | 0% | |
| 1,3-Dichlorobenzene | A | ug/L | 134.73853 | 5.3895412 | | 5 | 0 | 0 | 0.0803 | 0.5 | 500 | 108% | 80 | 119 | 0% | |
| 1,3-Dichloropropane | A | ug/L | 129.22354 | 5.1689416 | | 5 | 0 | 0 | 0.0791 | 0.5 | 500 | 103% | 80 | 119 | 0% | |
| 1,4-Dichlorobenzene | A | ug/L | 130.15948 | 5.2063792 | | 5 | 0 | 0 | 0.0858 | 0.5 | 500 | 104% | 79 | 118 | 0% | |
| 2,2-Dichloropropane | A | ug/L | 132.56709 | 5.3026836 | | 5 | 0 | 0 | 0.186 | 0.5 | 500 | 106% | 60 | 139 | 0% | |
| 2-Chlorotoluene | A | ug/L | 134.41808 | 5.3767232 | | 5 | 0 | 0 | 0.0876 | 0.5 | 500 | 108% | 79 | 122 | 0% | |
| 4-Chlorotoluene | A | ug/L | 136.3209 | 5.452836 | | 5 | 0 | 0 | 0.0728 | 0.5 | 500 | 109% | 78 | 122 | 0% | |
| Benzene | A | ug/L | 134.27415 | 5.370966 | | 5 | 0 | 0 | 0.0914 | 0.5 | 500 | 107% | 79 | 120 | 0% | |
| Bromobenzene | A | ug/L | 136.35762 | 5.4543048 | | 5 | 0 | 0 | 0.0831 | 0.5 | 500 | 109% | 80 | 120 | 0% | |
| Bromochloromethane | A | ug/L | 135.31234 | 5.4124936 | | 5 | 0 | 0 | 0.141 | 0.5 | 500 | 108% | 78 | 123 | 0% | |
| Bromodichloromethane | A | ug/L | 134.10931 | 5.3643724 | | 5 | 0 | 0 | 0.12 | 0.5 | 500 | 107% | 79 | 125 | 0% | |
| Bromoform | A | ug/L | 141.79502 | 5.6718008 | | 5 | 0 | 0 | 0.119 | 0.5 | 500 | 113% | 66 | 130 | 0% | |
| Bromomethane | A | ug/L | 109.56541 | 4.3826164 | | 5 | 0 | 0 | 0.253 | 0.5 | 500 | 88% | 53 | 141 | 0% | |
| Carbon tetrachloride | A | ug/L | 120.65262 | 4.8261048 | | 5 | 0 | 0 | 0.143 | 0.5 | 500 | 97% | 72 | 136 | 0% | |
| Chlorobenzene | A | ug/L | 132.50734 | 5.3002936 | | 5 | 0 | 0 | 0.0914 | 0.5 | 500 | 106% | 82 | 118 | 0% | |
| Chlorodibromomethane | A | ug/L | 132.59884 | 5.3039536 | | 5 | 0 | 0 | 0.0841 | 0.5 | 500 | 106% | 74 | 126 | 0% | |
| Chloroethane | A | ug/L | 115.63369 | 4.6253476 | | 5 | 0 | 0 | 0.169 | 0.5 | 500 | 93% | 60 | 138 | 0% | |
| Chloroform | A | ug/L | 123.16066 | 4.9264264 | | 5 | 0 | 0 | 0.0789 | 0.5 | 500 | 99% | 79 | 124 | 0% | |
| Chloromethane | A | ug/L | 112.36777 | 4.4947108 | | 5 | 0 | 0 | 0.162 | 0.5 | 500 | 90% | 50 | 139 | 0% | |
| cis-1,2-Dichloroethene | A | ug/L | 134.08788 | 5.3635152 | | 5 | 0 | 0 | 0.108 | 0.5 | 500 | 107% | 78 | 123 | 0% | |
| cis-1,3-Dichloropropene | A | ug/L | 125.62939 | 5.0251756 | | 5 | 0 | 0 | 0.073 | 0.5 | 500 | 101% | 75 | 124 | 0% | |
| Dibromomethane | A | ug/L | 130.25809 | 5.2103236 | | 5 | 0 | 0 | 0.147 | 0.5 | 500 | 104% | 79 | 123 | 0% | |
| Dichlorodifluoromethane | A | ug/L | 109.0928 | 4.363712 | | 5 | 0 | 0 | 0.175 | 0.5 | 500 | 87% | 32 | 152 | 0% | |
| Ethylbenzene | A | ug/L | 129.1693 | 5.166772 | | 5 | 0 | 0 | 0.0836 | 0.5 | 500 | 103% | 79 | 121 | 0% | |
| m+p-Xylenes | A | ug/L | 260.07995 | 10.403198 | | 10 | 0 | 0 | 0.15 | 0.5 | 1000 | 104% | 80 | 121 | 0% | |
| Methyl ethyl ketone | A | ug/L | 1303.70201 | 52.1480804 | | 50 | 0 | 0 | 1.77 | 10 | 5000 | 104% | 56 | 143 | 0% | |
| Methyl tert-butyl ether (MTBE) | A | ug/L | 143.1239 | 5.724956 | | 5 | 0 | 0 | 0.101 | 0.5 | 500 | 114% | 71 | 124 | 0% | |
| Methylene chloride | A | ug/L | 128.32091 | 5.1328364 | | 5 | 0 | 0 | 0.338 | 0.5 | 500 | 103% | 74 | 124 | 0% | |
| o-Xylene | A | ug/L | 131.27324 | 5.2509296 | | 5 | 0 | 0 | 0.0604 | 0.5 | 500 | 105% | 78 | 122 | 0% | |
| Styrene | A | ug/L | 135.16583 | 5.4066332 | | 5 | 0 | 0 | 0.067 | 0.5 | 500 | 108% | 78 | 123 | 0% | |
| Tetrachloroethene | A | ug/L | 127.47099 | 5.0988396 | | 5 | 0 | 0 | 0.0671 | 0.5 | 500 | 102% | 74 | 129 | 0% | |
| Toluene | A | ug/L | 134.40455 | 5.376182 | | 5 | 0 | 0 | 0.0679 | 0.5 | 500 | 108% | 80 | 121 | 0% | |
| trans-1,2-Dichloroethene | A | ug/L | 135.07074 | 5.4028296 | | 5 | 0 | 0 | 0.125 | 0.5 | 500 | 108% | 75 | 124 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971525 | LCS010522_ | VOC-8260-W-Q | LCS-DOD | DA5975C\VG010:1/5/2022 | 11:27:3 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| trans-1,3-Dichloropropene | A | ug/L | 138.03838 | 5.5215352 | | 5 | 0 | 0 | 0.0846 | 0.5 | 500 | 110% | 73 | 127 | 0% | |
| Trichloroethene | A | ug/L | 128.09371 | 5.1237484 | | 5 | 0 | 0 | 0.0993 | 0.5 | 500 | 102% | 79 | 123 | 0% | |
| Trichlorofluoromethane | A | ug/L | 123.94233 | 4.9576932 | | 5 | 0 | 0 | 0.134 | 0.5 | 500 | 99% | 65 | 141 | 0% | |
| Vinyl chloride | A | ug/L | 120.82943 | 4.8331772 | | 5 | 0 | 0 | 0.153 | 0.5 | 500 | 97% | 58 | 137 | 0% | |
| 1,4-Dichlorobenzene-d4 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 0 | 0 | 0% | |
| Chlorobenzene-d5 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 0 | 0 | 0% | |
| Fluorobenzene | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 0 | 0 | 0% | |
| Xylenes, Total | M | ug/L | 391.35319 | 15.6541276 | | 15 | 0 | 0 | 0.0604 | 0.5 | 1500 | 104% | 79 | 121 | 0% | |
| 1,2-Dichloroethane-d4 | S | ug/L | 282.23542 | 11.2894168 | | 10 | 0 | 0 | 0.229 | 0.5 | 500 | 113% | 81 | 118 | 0% | |
| Dibromofluoromethane | S | ug/L | 274.12732 | 10.9650928 | | 10 | 0 | 0 | 0.129 | 0.5 | 500 | 110% | 80 | 119 | 0% | |
| p-Bromofluorobenzene | S | ug/L | 269.64098 | 10.7856392 | | 10 | 0 | 0 | 0.149 | 0.5 | 500 | 108% | 85 | 114 | 0% | |
| Toluene-d8 | S | ug/L | 272.33887 | 10.8935548 | | 10 | 0 | 0 | 0.23 | 0.5 | 500 | 109% | 89 | 112 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|-------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971526 | MBLK010522_ | VOC-8260-W-Q | MBLK | DA5975C\VG010:1/5/2022 | 12:21:5 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 1,1,1-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.131 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 1,1,2,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0872 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 1,1,2-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 1,1-Dichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.135 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 1,1-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 1,1-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.083 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 1,2,3-Trichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.235 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 1,2-Dibromoethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0916 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 1,2-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0746 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 1,2-Dichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.116 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 1,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0847 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 1,3-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0803 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 1,3-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0791 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 1,4-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0858 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 2,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.186 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 2-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0876 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 4-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0728 | 0.5 | 500 | 0% | 0 | 0 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|--------------------------------|-------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971526 | MBLK010522_ | VOC-8260-W-Q | MBLK | DA5975CVVG010 | 1/5/2022 12:21:5 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| Benzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0914 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Bromobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0831 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Bromochloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Bromodichloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.12 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Bromoform | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.119 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Bromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.253 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Carbon tetrachloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.143 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Chlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0914 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Chlorodibromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0841 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Chloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.169 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Chloroform | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0789 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Chloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.162 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| cis-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| cis-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.073 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Dibromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.147 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Dichlorodifluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.175 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Ethylbenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0836 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| m+p-Xylenes | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.15 | 0.5 | 1000 | 0% | 0 | 0 | 0% | |
| Methyl ethyl ketone | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 1.77 | 10 | 5000 | 0% | 0 | 0 | 0% | |
| Methyl tert-butyl ether (MTBE) | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Methylene chloride | A | ug/L | 1.48861 | 0 | | 0 | 0 | 0 | 0.338 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| o-Xylene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0604 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Styrene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.067 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Tetrachloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0671 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Toluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0679 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| trans-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.125 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| trans-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0846 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Trichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0993 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Trichlorofluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.134 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Vinyl chloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.153 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| 1,4-Dichlorobenzene-d4 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 0 | 0 | 0% | |
| Chlorobenzene-d5 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 0 | 0 | 0% | |
| Fluorobenzene | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 0 | 0 | 0% | |
| Xylenes, Total | M | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0604 | 0.5 | 1500 | 0% | 0 | 0 | 0% | |
| 1,2-Dichloroethane-d4 | S | ug/L | 291.50907 | 11.6603628 | | 10 | 0 | 0 | 0.229 | 0.5 | 500 | 117% | 81 | 118 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|----------------------|-------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971526 | MBLK010522_ | VOC-8260-W-Q | MBLK | DA5975C\VG010:1/5/2022 | 12:21:5 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| Dibromofluoromethane | S | ug/L | 277.65061 | 11.1060244 | | 10 | 0 | 0 | 0.129 | 0.5 | 500 | 111% | 80 | 119 | 0% | |
| p-Bromofluorobenzene | S | ug/L | 263.93399 | 10.5573596 | | 10 | 0 | 0 | 0.149 | 0.5 | 500 | 106% | 85 | 114 | 0% | |
| Toluene-d8 | S | ug/L | 267.09011 | 10.6836044 | | 10 | 0 | 0 | 0.23 | 0.5 | 500 | 107% | 89 | 112 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|----------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971537 | B22010002-004 | VOC-8260-W-S | SAMP | DA5975C\VG010:1/5/2022 | 12:49:1 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971538 | B22010096-002 | VOC-8260-W-S | SAMP | DA5975C\VG010:1/5/2022 | 1:16:30 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,1-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.131 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,2,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0872 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,2-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.135 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.083 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2,3-Trichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.235 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dibromoethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0916 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0746 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.116 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0847 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,3-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0803 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,3-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0791 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,4-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0858 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 2,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.186 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 2-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0876 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 4-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0728 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Benzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0914 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0831 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromochloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 1 | 500 | 0% | 0 | 0 | 0% | U |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|--------------------------------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971538 | B22010096-002 | VOC-8260-W-S | SAMP | DA5975C\VG010:1/5/2022 | 1:16:30 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| Bromodichloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.12 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromoform | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.119 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.253 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Carbon tetrachloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.143 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0914 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chlorodibromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0841 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.169 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloroform | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0789 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloromethane | A | ug/L | 3.56369 | 0 | | 0 | 0 | 0 | 0.162 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| cis-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| cis-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.073 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Dibromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.147 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Dichlorodifluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.175 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Ethylbenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0836 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| m+p-Xylenes | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.15 | 1 | 1000 | 0% | 0 | 0 | 0% | U |
| Methyl ethyl ketone | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 1.77 | 20 | 5000 | 0% | 0 | 0 | 0% | U |
| Methyl tert-butyl ether (MTBE) | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Methylene chloride | A | ug/L | 1.63088 | 0 | | 0 | 0 | 0 | 0.338 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| o-Xylene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0604 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Styrene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.067 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Tetrachloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0671 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Toluene | A | ug/L | 0.90372 | 0 | | 0 | 0 | 0 | 0.0679 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| trans-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.125 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| trans-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0846 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Trichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0993 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Trichlorofluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.134 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Vinyl chloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.153 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,4-Dichlorobenzene-d4 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Chlorobenzene-d5 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0.1 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Fluorobenzene | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0.1 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Xylenes, Total | M | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0604 | 1 | 0 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloroethane-d4 | S | ug/L | 289.97834 | 11.5991336 | | 10 | 0 | 0 | 0.229 | 1 | 500 | 116% | 81 | 118 | 0% | |
| Dibromofluoromethane | S | ug/L | 279.85553 | 11.1942212 | | 10 | 0 | 0 | 0.129 | 1 | 500 | 112% | 80 | 119 | 0% | |
| p-Bromofluorobenzene | S | ug/L | 269.73697 | 10.7894788 | | 10 | 0 | 0 | 0.149 | 1 | 500 | 108% | 85 | 114 | 0% | |
| Toluene-d8 | S | ug/L | 264.72126 | 10.5888504 | | 10 | 0 | 0 | 0.23 | 1 | 500 | 106% | 89 | 112 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971539 | B22010120-002 | VOC-8260-W-S | SAMP | DA5975C\VG010:1/5/2022 | 1:43:48 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,1-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.131 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,2,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0872 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,2-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.135 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.083 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2,3-Trichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.235 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dibromoethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0916 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0746 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.116 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0847 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,3-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0803 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,3-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0791 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,4-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0858 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 2,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.186 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 2-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0876 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 4-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0728 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Benzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0914 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0831 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromochloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromodichloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.12 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromoform | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.119 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.253 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Carbon tetrachloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.143 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0914 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chlorodibromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0841 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.169 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloroform | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0789 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloromethane | A | ug/L | 3.49256 | 0 | | 0 | 0 | 0 | 0.162 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| cis-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| cis-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.073 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Dibromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.147 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Dichlorodifluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.175 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Ethylbenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0836 | 1 | 500 | 0% | 0 | 0 | 0% | U |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|--------------------------------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971539 | B22010120-002 | VOC-8260-W-S | SAMP | DA5975C\VG010:1/5/2022 | 1:43:48 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| m+p-Xylenes | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.15 | 1 | 1000 | 0% | 0 | 0 | 0% | U |
| Methyl ethyl ketone | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 1.77 | 20 | 5000 | 0% | 0 | 0 | 0% | U |
| Methyl tert-butyl ether (MTBE) | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Methylene chloride | A | ug/L | 1.7346 | 0 | | 0 | 0 | 0 | 0.338 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| o-Xylene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0604 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Styrene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.067 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Tetrachloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0671 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Toluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0679 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| trans-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.125 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| trans-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0846 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Trichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0993 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Trichlorofluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.134 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Vinyl chloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.153 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,4-Dichlorobenzene-d4 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Chlorobenzene-d5 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0.1 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Fluorobenzene | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0.1 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Xylenes, Total | M | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0604 | 1 | 0 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloroethane-d4 | S | ug/L | 295.94538 | 11.8378152 | | 10 | 0 | 0 | 0.229 | 1 | 500 | 118% | 81 | 118 | 0% | |
| Dibromofluoromethane | S | ug/L | 283.33331 | 11.3333324 | | 10 | 0 | 0 | 0.129 | 1 | 500 | 113% | 80 | 119 | 0% | |
| p-Bromofluorobenzene | S | ug/L | 268.54026 | 10.7416104 | | 10 | 0 | 0 | 0.149 | 1 | 500 | 107% | 85 | 114 | 0% | |
| Toluene-d8 | S | ug/L | 270.74611 | 10.8298444 | | 10 | 0 | 0 | 0.23 | 1 | 500 | 108% | 89 | 112 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971540 | B22010134-002 | VOC-8260-W-S | SAMP | DA5975C\VG010:1/5/2022 | 2:11:00 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,1-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.131 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,2,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0872 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,2-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.135 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.083 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2,3-Trichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.235 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dibromoethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0916 | 1 | 500 | 0% | 0 | 0 | 0% | U |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|--------------------------------|---------------|--------------|------------|-----------------|----------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971540 | B22010134-002 | VOC-8260-W-S | SAMP | DA5975C\VG010:1 | 5/2022 2:11:00 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,2-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0746 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.116 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0847 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,3-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0803 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,3-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0791 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,4-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0858 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 2,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.186 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 2-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0876 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 4-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0728 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Benzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0914 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0831 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromochloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromodichloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.12 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromoform | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.119 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.253 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Carbon tetrachloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.143 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0914 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chlorodibromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0841 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.169 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloroform | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0789 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloromethane | A | ug/L | 1.10028 | 0 | | 0 | 0 | 0 | 0.162 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| cis-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| cis-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.073 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Dibromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.147 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Dichlorodifluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.175 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Ethylbenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0836 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| m+p-Xylenes | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.15 | 1 | 1000 | 0% | 0 | 0 | 0% | U |
| Methyl ethyl ketone | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 1.77 | 20 | 5000 | 0% | 0 | 0 | 0% | U |
| Methyl tert-butyl ether (MTBE) | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Methylene chloride | A | ug/L | 1.15603 | 0 | | 0 | 0 | 0 | 0.338 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| o-Xylene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0604 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Styrene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.067 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Tetrachloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0671 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Toluene | A | ug/L | 0.86197 | 0 | | 0 | 0 | 0 | 0.0679 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| trans-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.125 | 1 | 500 | 0% | 0 | 0 | 0% | U |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|---------------|--------------|------------|--------------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971540 | B22010134-002 | VOC-8260-W-S | SAMP | DA5975C\VG010:1/5/2022 2:11:00 | | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| trans-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0846 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Trichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0993 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Trichlorofluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.134 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Vinyl chloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.153 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,4-Dichlorobenzene-d4 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Chlorobenzene-d5 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0.1 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Fluorobenzene | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0.1 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Xylenes, Total | M | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0604 | 1 | 0 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloroethane-d4 | S | ug/L | 286.86014 | 11.4744056 | | 10 | 0 | 0 | 0.229 | 1 | 500 | 115% | 81 | 118 | 0% | |
| Dibromofluoromethane | S | ug/L | 280.24166 | 11.2096664 | | 10 | 0 | 0 | 0.129 | 1 | 500 | 112% | 80 | 119 | 0% | |
| p-Bromofluorobenzene | S | ug/L | 275.01383 | 11.0005532 | | 10 | 0 | 0 | 0.149 | 1 | 500 | 110% | 85 | 114 | 0% | |
| Toluene-d8 | S | ug/L | 268.80887 | 10.7523548 | | 10 | 0 | 0 | 0.23 | 1 | 500 | 108% | 89 | 112 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|---------------|--------------|------------|--------------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971541 | B22010141-002 | VOC-8260-W-S | SAMP | DA5975C\VG010:1/5/2022 2:38:23 | | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,1-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.131 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,2,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0872 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,2-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.135 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.083 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2,3-Trichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.235 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dibromoethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0916 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0746 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.116 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0847 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,3-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0803 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,3-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0791 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,4-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0858 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 2,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.186 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 2-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0876 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 4-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0728 | 1 | 500 | 0% | 0 | 0 | 0% | U |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|--------------------------------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971541 | B22010141-002 | VOC-8260-W-S | SAMP | DA5975CVVG010:1/5/2022 | 2:38:23 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| Benzene | A | ug/L | 0.14752 | 0 | | 0 | 0 | 0 | 0.0914 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0831 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromochloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromodichloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.12 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromoform | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.119 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.253 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Carbon tetrachloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.143 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0914 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chlorodibromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0841 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.169 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloroform | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0789 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloromethane | A | ug/L | 1.27694 | 0 | | 0 | 0 | 0 | 0.162 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| cis-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| cis-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.073 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Dibromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.147 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Dichlorodifluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.175 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Ethylbenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0836 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| m+p-Xylenes | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.15 | 1 | 1000 | 0% | 0 | 0 | 0% | U |
| Methyl ethyl ketone | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 1.77 | 20 | 5000 | 0% | 0 | 0 | 0% | U |
| Methyl tert-butyl ether (MTBE) | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Methylene chloride | A | ug/L | 1.55165 | 0 | | 0 | 0 | 0 | 0.338 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| o-Xylene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0604 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Styrene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.067 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Tetrachloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0671 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Toluene | A | ug/L | 1.2239 | 0 | | 0 | 0 | 0 | 0.0679 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| trans-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.125 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| trans-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0846 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Trichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0993 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Trichlorofluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.134 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Vinyl chloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.153 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,4-Dichlorobenzene-d4 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Chlorobenzene-d5 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0.1 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Fluorobenzene | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0.1 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Xylenes, Total | M | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0604 | 1 | 0 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloroethane-d4 | S | ug/L | 291.48037 | 11.6592148 | | 10 | 0 | 0 | 0.229 | 1 | 500 | 117% | 81 | 118 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|----------------------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971541 | B22010141-002 | VOC-8260-W-S | SAMP | DA5975C\VG010:1/5/2022 | 2:38:23 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| Dibromofluoromethane | S | ug/L | 280.31885 | 11.212754 | | 10 | 0 | 0 | 0.129 | 1 | 500 | 112% | 80 | 119 | 0% | |
| p-Bromofluorobenzene | S | ug/L | 270.39993 | 10.8159972 | | 10 | 0 | 0 | 0.149 | 1 | 500 | 108% | 85 | 114 | 0% | |
| Toluene-d8 | S | ug/L | 267.76406 | 10.7105624 | | 10 | 0 | 0 | 0.23 | 1 | 500 | 107% | 89 | 112 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971542 | B22010142-002 | VOC-8260-W-S | SAMP | DA5975C\VG010:1/5/2022 | 3:05:50 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,1-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.131 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,2,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0872 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,2-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.135 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.083 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2,3-Trichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.235 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dibromoethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0916 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0746 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.116 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0847 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,3-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0803 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,3-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0791 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,4-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0858 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 2,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.186 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 2-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0876 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 4-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0728 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Benzene | A | ug/L | 0.14344 | 0 | | 0 | 0 | 0 | 0.0914 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0831 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromochloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromodichloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.12 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromoform | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.119 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.253 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Carbon tetrachloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.143 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0914 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chlorodibromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0841 | 1 | 500 | 0% | 0 | 0 | 0% | U |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|--------------------------------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971542 | B22010142-002 | VOC-8260-W-S | SAMP | DA5975C\VG010:1/5/2022 | 3:05:50 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| Chloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.169 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloroform | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0789 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloromethane | A | ug/L | 1.38074 | 0 | | 0 | 0 | 0 | 0.162 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| cis-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| cis-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.073 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Dibromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.147 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Dichlorodifluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.175 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Ethylbenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0836 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| m+p-Xylenes | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.15 | 1 | 1000 | 0% | 0 | 0 | 0% | U |
| Methyl ethyl ketone | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 1.77 | 20 | 5000 | 0% | 0 | 0 | 0% | U |
| Methyl tert-butyl ether (MTBE) | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Methylene chloride | A | ug/L | 2.21665 | 0 | | 0 | 0 | 0 | 0.338 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| o-Xylene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0604 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Styrene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.067 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Tetrachloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0671 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Toluene | A | ug/L | 1.5726 | 0 | | 0 | 0 | 0 | 0.0679 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| trans-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.125 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| trans-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0846 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Trichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0993 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Trichlorofluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.134 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Vinyl chloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.153 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,4-Dichlorobenzene-d4 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Chlorobenzene-d5 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0.1 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Fluorobenzene | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0.1 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Xylenes, Total | M | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0604 | 1 | 0 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloroethane-d4 | S | ug/L | 288.47239 | 11.5388956 | | 10 | 0 | 0 | 0.229 | 1 | 500 | 115% | 81 | 118 | 0% | |
| Dibromofluoromethane | S | ug/L | 285.77548 | 11.4310192 | | 10 | 0 | 0 | 0.129 | 1 | 500 | 114% | 80 | 119 | 0% | |
| p-Bromofluorobenzene | S | ug/L | 271.31161 | 10.8524644 | | 10 | 0 | 0 | 0.149 | 1 | 500 | 109% | 85 | 114 | 0% | |
| Toluene-d8 | S | ug/L | 267.22171 | 10.6888684 | | 10 | 0 | 0 | 0.23 | 1 | 500 | 107% | 89 | 112 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|----------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971543 | B22010143-002 | VOC-8260-W-S | SAMP | DA5975C\VG010:1/5/2022 | 3:33:12 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971543 | B22010143-002 | VOC-8260-W-S | SAMP | DA5975C\VG010:1/5/2022 | 3:33:12 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,1-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.131 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,2,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0872 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,2-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.135 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.083 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2,3-Trichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.235 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dibromoethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0916 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0746 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.116 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0847 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,3-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0803 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,3-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0791 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,4-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0858 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 2,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.186 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 2-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0876 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 4-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0728 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Benzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0914 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0831 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromochloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromodichloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.12 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromoform | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.119 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.253 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Carbon tetrachloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.143 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0914 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chlorodibromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0841 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.169 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloroform | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0789 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloromethane | A | ug/L | 0.82227 | 0 | | 0 | 0 | 0 | 0.162 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| cis-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| cis-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.073 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Dibromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.147 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Dichlorodifluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.175 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Ethylbenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0836 | 1 | 500 | 0% | 0 | 0 | 0% | U |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|--------------------------------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971543 | B22010143-002 | VOC-8260-W-S | SAMP | DA5975C\VG010:1/5/2022 | 3:33:12 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| m+p-Xylenes | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.15 | 1 | 1000 | 0% | 0 | 0 | 0% | U |
| Methyl ethyl ketone | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 1.77 | 20 | 5000 | 0% | 0 | 0 | 0% | U |
| Methyl tert-butyl ether (MTBE) | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Methylene chloride | A | ug/L | 1.69772 | 0 | | 0 | 0 | 0 | 0.338 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| o-Xylene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0604 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Styrene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.067 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Tetrachloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0671 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Toluene | A | ug/L | 1.63082 | 0 | | 0 | 0 | 0 | 0.0679 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| trans-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.125 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| trans-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0846 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Trichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0993 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Trichlorofluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.134 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Vinyl chloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.153 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,4-Dichlorobenzene-d4 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Chlorobenzene-d5 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0.1 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Fluorobenzene | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0.1 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Xylenes, Total | M | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0604 | 1 | 0 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloroethane-d4 | S | ug/L | 281.18364 | 11.2473456 | | 10 | 0 | 0 | 0.229 | 1 | 500 | 112% | 81 | 118 | 0% | |
| Dibromofluoromethane | S | ug/L | 278.74321 | 11.1497284 | | 10 | 0 | 0 | 0.129 | 1 | 500 | 111% | 80 | 119 | 0% | |
| p-Bromofluorobenzene | S | ug/L | 265.34242 | 10.6136968 | | 10 | 0 | 0 | 0.149 | 1 | 500 | 106% | 85 | 114 | 0% | |
| Toluene-d8 | S | ug/L | 266.87328 | 10.6749312 | | 10 | 0 | 0 | 0.23 | 1 | 500 | 107% | 89 | 112 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971544 | B22010002-001 | VOC-8260-W-S | SAMP | DA5975C\VG010:1/5/2022 | 4:00:32 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,1-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.131 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,2,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0872 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,2-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.135 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.083 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2,3-Trichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.235 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dibromoethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0916 | 1 | 500 | 0% | 0 | 0 | 0% | U |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|--------------------------------|---------------|--------------|------------|-----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971544 | B22010002-001 | VOC-8260-W-S | SAMP | DA5975C\VG010:1 | 1/5/2022 4:00:32 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,2-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0746 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.116 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0847 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,3-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0803 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,3-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0791 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,4-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0858 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 2,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.186 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 2-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0876 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 4-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0728 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Benzene | A | ug/L | 0.12664 | 0 | | 0 | 0 | 0 | 0.0914 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0831 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromochloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromodichloromethane | A | ug/L | 1.63533 | 0 | | 0 | 0 | 0 | 0.12 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromoform | A | ug/L | 16.54828 | 0.6619312 | | 0 | 0 | 0 | 0.119 | 1 | 500 | 0% | 0 | 0 | 0% | J |
| Bromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.253 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Carbon tetrachloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.143 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0914 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chlorodibromomethane | A | ug/L | 5.79504 | 0.2318016 | | 0 | 0 | 0 | 0.0841 | 1 | 500 | 0% | 0 | 0 | 0% | J |
| Chloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.169 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloroform | A | ug/L | 1.90539 | 0 | | 0 | 0 | 0 | 0.0789 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloromethane | A | ug/L | 0.54328 | 0 | | 0 | 0 | 0 | 0.162 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| cis-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| cis-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.073 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Dibromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.147 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Dichlorodifluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.175 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Ethylbenzene | A | ug/L | 0.09654 | 0 | | 0 | 0 | 0 | 0.0836 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| m+p-Xylenes | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.15 | 1 | 1000 | 0% | 0 | 0 | 0% | U |
| Methyl ethyl ketone | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 1.77 | 20 | 5000 | 0% | 0 | 0 | 0% | U |
| Methyl tert-butyl ether (MTBE) | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Methylene chloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.338 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| o-Xylene | A | ug/L | 2.13119 | 0.0852476 | | 0 | 0 | 0 | 0.0604 | 1 | 500 | 0% | 0 | 0 | 0% | J |
| Styrene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.067 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Tetrachloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0671 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Toluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0679 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| trans-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.125 | 1 | 500 | 0% | 0 | 0 | 0% | U |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971544 | B22010002-001 | VOC-8260-W-S | SAMP | DA5975C\VG010:1/5/2022 | 4:00:32 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| trans-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0846 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Trichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0993 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Trichlorofluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.134 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Vinyl chloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.153 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,4-Dichlorobenzene-d4 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Chlorobenzene-d5 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0.1 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Fluorobenzene | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0.1 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Xylenes, Total | M | ug/L | 2.13119 | 0.0852476 | | 0 | 0 | 0 | 0.0604 | 1 | 0 | 0% | 0 | 0 | 0% | J |
| 1,2-Dichloroethane-d4 | S | ug/L | 295.27075 | 11.81083 | | 10 | 0 | 0 | 0.229 | 1 | 500 | 118% | 81 | 118 | 0% | |
| Dibromofluoromethane | S | ug/L | 278.55532 | 11.1422128 | | 10 | 0 | 0 | 0.129 | 1 | 500 | 111% | 80 | 119 | 0% | |
| p-Bromofluorobenzene | S | ug/L | 264.11239 | 10.5644956 | | 10 | 0 | 0 | 0.149 | 1 | 500 | 106% | 85 | 114 | 0% | |
| Toluene-d8 | S | ug/L | 264.08962 | 10.5635848 | | 10 | 0 | 0 | 0.23 | 1 | 500 | 106% | 89 | 112 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971545 | B22010002-002 | VOC-8260-W-S | SAMP | DA5975C\VG010:1/5/2022 | 4:27:50 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,1-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.131 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,2,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0872 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,2-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.135 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.083 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2,3-Trichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.235 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dibromoethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0916 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0746 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.116 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0847 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,3-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0803 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,3-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0791 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,4-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0858 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 2,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.186 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 2-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0876 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 4-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0728 | 1 | 500 | 0% | 0 | 0 | 0% | U |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|--------------------------------|---------------|--------------|------------|-----------------|----------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971545 | B22010002-002 | VOC-8260-W-S | SAMP | DA5975C\VG010:1 | 5/2022 4:27:50 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| Benzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0914 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0831 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromochloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromodichloromethane | A | ug/L | 1.89432 | 0 | | 0 | 0 | 0 | 0.12 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromoform | A | ug/L | 15.37295 | 0.614918 | | 0 | 0 | 0 | 0.119 | 1 | 500 | 0% | 0 | 0 | 0% | J |
| Bromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.253 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Carbon tetrachloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.143 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0914 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chlorodibromomethane | A | ug/L | 5.20758 | 0.2083032 | | 0 | 0 | 0 | 0.0841 | 1 | 500 | 0% | 0 | 0 | 0% | J |
| Chloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.169 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloroform | A | ug/L | 1.90877 | 0 | | 0 | 0 | 0 | 0.0789 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloromethane | A | ug/L | 0.44409 | 0 | | 0 | 0 | 0 | 0.162 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| cis-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| cis-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.073 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Dibromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.147 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Dichlorodifluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.175 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Ethylbenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0836 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| m+p-Xylenes | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.15 | 1 | 1000 | 0% | 0 | 0 | 0% | U |
| Methyl ethyl ketone | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 1.77 | 20 | 5000 | 0% | 0 | 0 | 0% | U |
| Methyl tert-butyl ether (MTBE) | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Methylene chloride | A | ug/L | 0.59257 | 0 | | 0 | 0 | 0 | 0.338 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| o-Xylene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0604 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Styrene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.067 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Tetrachloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0671 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Toluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0679 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| trans-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.125 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| trans-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0846 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Trichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0993 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Trichlorofluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.134 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Vinyl chloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.153 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,4-Dichlorobenzene-d4 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Chlorobenzene-d5 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0.1 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Fluorobenzene | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0.1 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Xylenes, Total | M | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0604 | 1 | 0 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloroethane-d4 | S | ug/L | 289.1908 | 11.567632 | | 10 | 0 | 0 | 0.229 | 1 | 500 | 116% | 81 | 118 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|----------------------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971545 | B22010002-002 | VOC-8260-W-S | SAMP | DA5975C\VG010:1/5/2022 | 4:27:50 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| Dibromofluoromethane | S | ug/L | 277.68068 | 11.1072272 | | 10 | 0 | 0 | 0.129 | 1 | 500 | 111% | 80 | 119 | 0% | |
| p-Bromofluorobenzene | S | ug/L | 270.80782 | 10.8323128 | | 10 | 0 | 0 | 0.149 | 1 | 500 | 108% | 85 | 114 | 0% | |
| Toluene-d8 | S | ug/L | 265.93701 | 10.6374804 | | 10 | 0 | 0 | 0.23 | 1 | 500 | 106% | 89 | 112 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971546 | B22010002-003 | VOC-8260-W-S | SAMP | DA5975C\VG010:1/5/2022 | 4:55:12 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,1-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.131 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,2,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0872 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,2-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.135 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.083 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2,3-Trichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.235 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dibromoethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0916 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0746 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.116 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0847 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,3-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0803 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,3-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0791 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,4-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0858 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 2,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.186 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 2-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0876 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 4-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0728 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Benzene | A | ug/L | 0.14657 | 0 | | 0 | 0 | 0 | 0.0914 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0831 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromochloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromodichloromethane | A | ug/L | 2.08157 | 0 | | 0 | 0 | 0 | 0.12 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromoform | A | ug/L | 16.35591 | 0.6542364 | | 0 | 0 | 0 | 0.119 | 1 | 500 | 0% | 0 | 0 | 0% | J |
| Bromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.253 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Carbon tetrachloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.143 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0914 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chlorodibromomethane | A | ug/L | 5.74957 | 0.2299828 | | 0 | 0 | 0 | 0.0841 | 1 | 500 | 0% | 0 | 0 | 0% | J |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|--------------------------------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971546 | B22010002-003 | VOC-8260-W-S | SAMP | DA5975C\VG010:1/5/2022 | 4:55:12 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| Chloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.169 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloroform | A | ug/L | 1.70841 | 0 | | 0 | 0 | 0 | 0.0789 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloromethane | A | ug/L | 4.0503 | 0.162012 | | 0 | 0 | 0 | 0.162 | 1 | 500 | 0% | 0 | 0 | 0% | J |
| cis-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| cis-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.073 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Dibromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.147 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Dichlorodifluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.175 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Ethylbenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0836 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| m+p-Xylenes | A | ug/L | 0.4778 | 0 | | 0 | 0 | 0 | 0.15 | 1 | 1000 | 0% | 0 | 0 | 0% | U |
| Methyl ethyl ketone | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 1.77 | 20 | 5000 | 0% | 0 | 0 | 0% | U |
| Methyl tert-butyl ether (MTBE) | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Methylene chloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.338 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| o-Xylene | A | ug/L | 1.19898 | 0 | | 0 | 0 | 0 | 0.0604 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Styrene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.067 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Tetrachloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0671 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Toluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0679 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| trans-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.125 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| trans-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0846 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Trichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0993 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Trichlorofluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.134 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Vinyl chloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.153 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,4-Dichlorobenzene-d4 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Chlorobenzene-d5 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0.1 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Fluorobenzene | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0.1 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Xylenes, Total | M | ug/L | 1.67678 | 0.0670712 | | 0 | 0 | 0 | 0.0604 | 1 | 0 | 0% | 0 | 0 | 0% | J |
| 1,2-Dichloroethane-d4 | S | ug/L | 284.63077 | 11.3852308 | | 10 | 0 | 0 | 0.229 | 1 | 500 | 114% | 81 | 118 | 0% | |
| Dibromofluoromethane | S | ug/L | 276.66529 | 11.0666116 | | 10 | 0 | 0 | 0.129 | 1 | 500 | 111% | 80 | 119 | 0% | |
| p-Bromofluorobenzene | S | ug/L | 264.52391 | 10.5809564 | | 10 | 0 | 0 | 0.149 | 1 | 500 | 106% | 85 | 114 | 0% | |
| Toluene-d8 | S | ug/L | 265.62246 | 10.6248984 | | 10 | 0 | 0 | 0.23 | 1 | 500 | 106% | 89 | 112 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|----------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971547 | B22010096-001 | VOC-8260-W-S | SAMP | DA5975C\VG010:1/5/2022 | 5:22:23 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|---------------|--------------|------------|-----------------|----------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971547 | B22010096-001 | VOC-8260-W-S | SAMP | DA5975C\VG010:1 | 5/2022 5:22:23 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,1-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.131 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,2,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0872 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,2-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.135 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.083 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2,3-Trichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.235 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dibromoethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0916 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0746 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.116 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0847 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,3-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0803 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,3-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0791 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,4-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0858 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 2,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.186 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 2-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0876 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 4-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0728 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Benzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0914 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0831 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromochloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromodichloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.12 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromoform | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.119 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.253 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Carbon tetrachloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.143 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0914 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chlorodibromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0841 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.169 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloroform | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0789 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloromethane | A | ug/L | 0.88371 | 0 | | 0 | 0 | 0 | 0.162 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| cis-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| cis-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.073 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Dibromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.147 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Dichlorodifluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.175 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Ethylbenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0836 | 1 | 500 | 0% | 0 | 0 | 0% | U |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|--------------------------------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971547 | B22010096-001 | VOC-8260-W-S | SAMP | DA5975C\VG010:1/5/2022 | 5:22:23 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| m+p-Xylenes | A | ug/L | 0.04631 | 0 | | 0 | 0 | 0 | 0.15 | 1 | 1000 | 0% | 0 | 0 | 0% | U |
| Methyl ethyl ketone | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 1.77 | 20 | 5000 | 0% | 0 | 0 | 0% | U |
| Methyl tert-butyl ether (MTBE) | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Methylene chloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.338 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| o-Xylene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0604 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Styrene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.067 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Tetrachloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0671 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Toluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0679 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| trans-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.125 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| trans-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0846 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Trichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0993 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Trichlorofluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.134 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Vinyl chloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.153 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,4-Dichlorobenzene-d4 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Chlorobenzene-d5 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0.1 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Fluorobenzene | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0.1 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Xylenes, Total | M | ug/L | 0.04631 | 0 | | 0 | 0 | 0 | 0.0604 | 1 | 0 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloroethane-d4 | S | ug/L | 287.70198 | 11.5080792 | | 10 | 0 | 0 | 0.229 | 1 | 500 | 115% | 81 | 118 | 0% | |
| Dibromofluoromethane | S | ug/L | 278.05136 | 11.1220544 | | 10 | 0 | 0 | 0.129 | 1 | 500 | 111% | 80 | 119 | 0% | |
| p-Bromofluorobenzene | S | ug/L | 272.22777 | 10.8891108 | | 10 | 0 | 0 | 0.149 | 1 | 500 | 109% | 85 | 114 | 0% | |
| Toluene-d8 | S | ug/L | 270.87613 | 10.8350452 | | 10 | 0 | 0 | 0.23 | 1 | 500 | 108% | 89 | 112 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971548 | B22010120-001 | VOC-8260-W-S | SAMP | DA5975C\VG010:1/5/2022 | 5:49:37 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,1-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.131 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,2,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0872 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,2-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.135 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.083 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2,3-Trichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.235 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dibromoethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0916 | 1 | 500 | 0% | 0 | 0 | 0% | U |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|--------------------------------|---------------|--------------|------------|-----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971548 | B22010120-001 | VOC-8260-W-S | SAMP | DA5975C\VG010:1 | 1/5/2022 5:49:37 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,2-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0746 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloroethane | A | ug/L | 6.00028 | 0.2400112 | | 0 | 0 | 0 | 0.116 | 1 | 500 | 0% | 0 | 0 | 0% | J |
| 1,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0847 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,3-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0803 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,3-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0791 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,4-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0858 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 2,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.186 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 2-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0876 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 4-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0728 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Benzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0914 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0831 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromochloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromodichloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.12 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromoform | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.119 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.253 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Carbon tetrachloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.143 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0914 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chlorodibromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0841 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.169 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloroform | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0789 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.162 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| cis-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| cis-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.073 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Dibromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.147 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Dichlorodifluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.175 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Ethylbenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0836 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| m+p-Xylenes | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.15 | 1 | 1000 | 0% | 0 | 0 | 0% | U |
| Methyl ethyl ketone | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 1.77 | 20 | 5000 | 0% | 0 | 0 | 0% | U |
| Methyl tert-butyl ether (MTBE) | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Methylene chloride | A | ug/L | 0.42097 | 0 | | 0 | 0 | 0 | 0.338 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| o-Xylene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0604 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Styrene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.067 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Tetrachloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0671 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Toluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0679 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| trans-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.125 | 1 | 500 | 0% | 0 | 0 | 0% | U |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971548 | B22010120-001 | VOC-8260-W-S | SAMP | DA5975C\VG010:1/5/2022 | 5:49:37 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| trans-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0846 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Trichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0993 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Trichlorofluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.134 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Vinyl chloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.153 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,4-Dichlorobenzene-d4 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Chlorobenzene-d5 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0.1 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Fluorobenzene | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0.1 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Xylenes, Total | M | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0604 | 1 | 0 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloroethane-d4 | S | ug/L | 293.31496 | 11.7325984 | | 10 | 0 | 0 | 0.229 | 1 | 500 | 117% | 81 | 118 | 0% | |
| Dibromofluoromethane | S | ug/L | 277.61341 | 11.1045364 | | 10 | 0 | 0 | 0.129 | 1 | 500 | 111% | 80 | 119 | 0% | |
| p-Bromofluorobenzene | S | ug/L | 266.8629 | 10.674516 | | 10 | 0 | 0 | 0.149 | 1 | 500 | 107% | 85 | 114 | 0% | |
| Toluene-d8 | S | ug/L | 269.93541 | 10.7974164 | | 10 | 0 | 0 | 0.23 | 1 | 500 | 108% | 89 | 112 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971549 | B22010134-001 | VOC-8260-W-S | SAMP | DA5975C\VG010:1/5/2022 | 6:16:51 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,1-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.131 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,2,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0872 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,2-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.135 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.083 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2,3-Trichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.235 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dibromoethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0916 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0746 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.116 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0847 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,3-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0803 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,3-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0791 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,4-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0858 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 2,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.186 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 2-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0876 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 4-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0728 | 1 | 500 | 0% | 0 | 0 | 0% | U |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|--------------------------------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971549 | B22010134-001 | VOC-8260-W-S | SAMP | DA5975CVVG010:1/5/2022 | 6:16:51 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| Benzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0914 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0831 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromochloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromodichloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.12 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromoform | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.119 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.253 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Carbon tetrachloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.143 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0914 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chlorodibromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0841 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.169 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloroform | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0789 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloromethane | A | ug/L | 1.16528 | 0 | | 0 | 0 | 0 | 0.162 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| cis-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| cis-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.073 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Dibromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.147 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Dichlorodifluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.175 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Ethylbenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0836 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| m+p-Xylenes | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.15 | 1 | 1000 | 0% | 0 | 0 | 0% | U |
| Methyl ethyl ketone | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 1.77 | 20 | 5000 | 0% | 0 | 0 | 0% | U |
| Methyl tert-butyl ether (MTBE) | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Methylene chloride | A | ug/L | 0.69364 | 0 | | 0 | 0 | 0 | 0.338 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| o-Xylene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0604 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Styrene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.067 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Tetrachloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0671 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Toluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0679 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| trans-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.125 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| trans-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0846 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Trichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0993 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Trichlorofluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.134 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Vinyl chloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.153 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,4-Dichlorobenzene-d4 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Chlorobenzene-d5 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0.1 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Fluorobenzene | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0.1 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Xylenes, Total | M | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0604 | 1 | 0 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloroethane-d4 | S | ug/L | 284.90915 | 11.396366 | | 10 | 0 | 0 | 0.229 | 1 | 500 | 114% | 81 | 118 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|----------------------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971549 | B22010134-001 | VOC-8260-W-S | SAMP | DA5975C\VG010:1/5/2022 | 6:16:51 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| Dibromofluoromethane | S | ug/L | 281.03574 | 11.2414296 | | 10 | 0 | 0 | 0.129 | 1 | 500 | 112% | 80 | 119 | 0% | |
| p-Bromofluorobenzene | S | ug/L | 269.49342 | 10.7797368 | | 10 | 0 | 0 | 0.149 | 1 | 500 | 108% | 85 | 114 | 0% | |
| Toluene-d8 | S | ug/L | 268.66914 | 10.7467656 | | 10 | 0 | 0 | 0.23 | 1 | 500 | 107% | 89 | 112 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971550 | B22010141-001 | VOC-8260-W-S | SAMP | DA5975C\VG010:1/5/2022 | 6:44:10 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,1-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.131 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,2,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0872 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,2-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.135 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.083 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2,3-Trichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.235 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dibromoethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0916 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0746 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.116 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0847 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,3-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0803 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,3-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0791 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,4-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0858 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 2,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.186 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 2-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0876 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 4-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0728 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Benzene | A | ug/L | 0.14554 | 0 | | 0 | 0 | 0 | 0.0914 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0831 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromochloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromodichloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.12 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromoform | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.119 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.253 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Carbon tetrachloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.143 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0914 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chlorodibromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0841 | 1 | 500 | 0% | 0 | 0 | 0% | U |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|--------------------------------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971550 | B22010141-001 | VOC-8260-W-S | SAMP | DA5975C\VG010:1/5/2022 | 6:44:10 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| Chloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.169 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloroform | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0789 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.162 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| cis-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| cis-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.073 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Dibromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.147 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Dichlorodifluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.175 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Ethylbenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0836 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| m+p-Xylenes | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.15 | 1 | 1000 | 0% | 0 | 0 | 0% | U |
| Methyl ethyl ketone | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 1.77 | 20 | 5000 | 0% | 0 | 0 | 0% | U |
| Methyl tert-butyl ether (MTBE) | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Methylene chloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.338 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| o-Xylene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0604 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Styrene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.067 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Tetrachloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0671 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Toluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0679 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| trans-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.125 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| trans-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0846 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Trichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0993 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Trichlorofluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.134 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Vinyl chloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.153 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,4-Dichlorobenzene-d4 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Chlorobenzene-d5 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0.1 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Fluorobenzene | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0.1 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Xylenes, Total | M | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0604 | 1 | 0 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloroethane-d4 | S | ug/L | 287.12367 | 11.4849468 | | 10 | 0 | 0 | 0.229 | 1 | 500 | 115% | 81 | 118 | 0% | |
| Dibromofluoromethane | S | ug/L | 277.49716 | 11.0998864 | | 10 | 0 | 0 | 0.129 | 1 | 500 | 111% | 80 | 119 | 0% | |
| p-Bromofluorobenzene | S | ug/L | 265.61597 | 10.6246388 | | 10 | 0 | 0 | 0.149 | 1 | 500 | 106% | 85 | 114 | 0% | |
| Toluene-d8 | S | ug/L | 266.98971 | 10.6795884 | | 10 | 0 | 0 | 0.23 | 1 | 500 | 107% | 89 | 112 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|----------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971551 | B22010142-001 | VOC-8260-W-S | SAMP | DA5975C\VG010:1/5/2022 | 7:11:33 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971551 | B22010142-001 | VOC-8260-W-S | SAMP | DA5975C\VG010:1/5/2022 | 7:11:33 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,1-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.131 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,2,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0872 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,2-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.135 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.083 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2,3-Trichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.235 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dibromoethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0916 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0746 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.116 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0847 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,3-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0803 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,3-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0791 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,4-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0858 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 2,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.186 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 2-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0876 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 4-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0728 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Benzene | A | ug/L | 0.09675 | 0 | | 0 | 0 | 0 | 0.0914 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0831 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromochloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromodichloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.12 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromoform | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.119 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.253 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Carbon tetrachloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.143 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0914 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chlorodibromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0841 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.169 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloroform | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0789 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloromethane | A | ug/L | 1.55746 | 0 | | 0 | 0 | 0 | 0.162 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| cis-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| cis-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.073 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Dibromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.147 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Dichlorodifluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.175 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Ethylbenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0836 | 1 | 500 | 0% | 0 | 0 | 0% | U |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|--------------------------------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971551 | B22010142-001 | VOC-8260-W-S | SAMP | DA5975C\VG010:1/5/2022 | 7:11:33 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| m+p-Xylenes | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.15 | 1 | 1000 | 0% | 0 | 0 | 0% | U |
| Methyl ethyl ketone | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 1.77 | 20 | 5000 | 0% | 0 | 0 | 0% | U |
| Methyl tert-butyl ether (MTBE) | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Methylene chloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.338 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| o-Xylene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0604 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Styrene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.067 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Tetrachloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0671 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Toluene | A | ug/L | 1.19327 | 0 | | 0 | 0 | 0 | 0.0679 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| trans-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.125 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| trans-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0846 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Trichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0993 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Trichlorofluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.134 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Vinyl chloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.153 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,4-Dichlorobenzene-d4 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Chlorobenzene-d5 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0.1 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Fluorobenzene | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0.1 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Xylenes, Total | M | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0604 | 1 | 0 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloroethane-d4 | S | ug/L | 294.78953 | 11.7915812 | | 10 | 0 | 0 | 0.229 | 1 | 500 | 118% | 81 | 118 | 0% | |
| Dibromofluoromethane | S | ug/L | 282.3413 | 11.293652 | | 10 | 0 | 0 | 0.129 | 1 | 500 | 113% | 80 | 119 | 0% | |
| p-Bromofluorobenzene | S | ug/L | 271.12478 | 10.8449912 | | 10 | 0 | 0 | 0.149 | 1 | 500 | 108% | 85 | 114 | 0% | |
| Toluene-d8 | S | ug/L | 266.12067 | 10.6448268 | | 10 | 0 | 0 | 0.23 | 1 | 500 | 106% | 89 | 112 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971552 | B22010143-001 | VOC-8260-W-S | SAMP | DA5975C\VG010:1/5/2022 | 7:38:52 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,1-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.131 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,2,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0872 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,2-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.135 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.083 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2,3-Trichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.235 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dibromoethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0916 | 1 | 500 | 0% | 0 | 0 | 0% | U |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|--------------------------------|---------------|--------------|------------|-----------------|----------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971552 | B22010143-001 | VOC-8260-W-S | SAMP | DA5975C\VG010:1 | 5/2022 7:38:52 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,2-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0746 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.116 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0847 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,3-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0803 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,3-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0791 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,4-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0858 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 2,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.186 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 2-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0876 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 4-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0728 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Benzene | A | ug/L | 0.63949 | 0 | | 0 | 0 | 0 | 0.0914 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0831 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromochloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromodichloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.12 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromoform | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.119 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Bromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.253 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Carbon tetrachloride | A | ug/L | 1.00552 | 0 | | 0 | 0 | 0 | 0.143 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0914 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chlorodibromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0841 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloroethane | A | ug/L | 3.26204 | 0 | | 0 | 0 | 0 | 0.169 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloroform | A | ug/L | 52.21756 | 2.0887024 | | 0 | 0 | 0 | 0.0789 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Chloromethane | A | ug/L | 3.23447 | 0 | | 0 | 0 | 0 | 0.162 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| cis-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| cis-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.073 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Dibromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.147 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Dichlorodifluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.175 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Ethylbenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0836 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| m+p-Xylenes | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.15 | 1 | 1000 | 0% | 0 | 0 | 0% | U |
| Methyl ethyl ketone | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 1.77 | 20 | 5000 | 0% | 0 | 0 | 0% | U |
| Methyl tert-butyl ether (MTBE) | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Methylene chloride | A | ug/L | 1.02328 | 0 | | 0 | 0 | 0 | 0.338 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| o-Xylene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0604 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Styrene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.067 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Tetrachloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0671 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Toluene | A | ug/L | 0.14142 | 0 | | 0 | 0 | 0 | 0.0679 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| trans-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.125 | 1 | 500 | 0% | 0 | 0 | 0% | U |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971552 | B22010143-001 | VOC-8260-W-S | SAMP | DA5975C\VG010:1/5/2022 | 7:38:52 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| trans-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0846 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Trichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0993 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Trichlorofluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.134 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| Vinyl chloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.153 | 1 | 500 | 0% | 0 | 0 | 0% | U |
| 1,4-Dichlorobenzene-d4 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Chlorobenzene-d5 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0.1 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Fluorobenzene | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0.1 | 0 | 0 | 0% | 0 | 0 | 0% | |
| Xylenes, Total | M | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0604 | 1 | 0 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloroethane-d4 | S | ug/L | 287.76422 | 11.5105688 | | 10 | 0 | 0 | 0.229 | 1 | 500 | 115% | 81 | 118 | 0% | |
| Dibromofluoromethane | S | ug/L | 282.74626 | 11.3098504 | | 10 | 0 | 0 | 0.129 | 1 | 500 | 113% | 80 | 119 | 0% | |
| p-Bromofluorobenzene | S | ug/L | 270.11863 | 10.8047452 | | 10 | 0 | 0 | 0.149 | 1 | 500 | 108% | 85 | 114 | 0% | |
| Toluene-d8 | S | ug/L | 264.64337 | 10.5857348 | | 10 | 0 | 0 | 0.23 | 1 | 500 | 106% | 89 | 112 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971553 | B22010002-001 | VOC-8260-W-Q | SAMP | DA5975C\VG010:1/5/2022 | 4:00:32 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,1-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.131 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,2,2-Tetrachloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0872 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1,2-Trichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.135 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| 1,1-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.083 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2,3-Trichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.235 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dibromoethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0916 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0746 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.116 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| 1,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0847 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| 1,3-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0803 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| 1,3-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0791 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| 1,4-Dichlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0858 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| 2,2-Dichloropropane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.186 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| 2-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0876 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| 4-Chlorotoluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0728 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|--------------------------------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971553 | B22010002-001 | VOC-8260-W-Q | SAMP | DA5975C\VG010:1/5/2022 | 4:00:32 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| Benzene | A | ug/L | 0.12664 | 0 | | 0 | 0 | 0 | 0.0914 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| Bromobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0831 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| Bromochloromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.141 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| Bromodichloromethane | A | ug/L | 1.63533 | 0 | | 0 | 0 | 0 | 0.12 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| Bromoform | A | ug/L | 16.54828 | 0.6619312 | | 0 | 0 | 0 | 0.119 | 0.5 | 500 | 0% | 0 | 0 | 0% | |
| Bromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.253 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| Carbon tetrachloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.143 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| Chlorobenzene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0914 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| Chlorodibromomethane | A | ug/L | 5.79504 | 0.2318016 | | 0 | 0 | 0 | 0.0841 | 0.5 | 500 | 0% | 0 | 0 | 0% | J |
| Chloroethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.169 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| Chloroform | A | ug/L | 1.90539 | 0 | | 0 | 0 | 0 | 0.0789 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| Chloromethane | A | ug/L | 0.54328 | 0 | | 0 | 0 | 0 | 0.162 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| cis-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.108 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| cis-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.073 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| Dibromomethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.147 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| Dichlorodifluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.175 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| Ethylbenzene | A | ug/L | 0.09654 | 0 | | 0 | 0 | 0 | 0.0836 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| m+p-Xylenes | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.15 | 0.5 | 1000 | 0% | 0 | 0 | 0% | U |
| Methyl ethyl ketone | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 1.77 | 10 | 5000 | 0% | 0 | 0 | 0% | U |
| Methyl tert-butyl ether (MTBE) | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.101 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| Methylene chloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.338 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| o-Xylene | A | ug/L | 2.13119 | 0.0852476 | | 0 | 0 | 0 | 0.0604 | 0.5 | 500 | 0% | 0 | 0 | 0% | J |
| Styrene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.067 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| Tetrachloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0671 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| Toluene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0679 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| trans-1,2-Dichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.125 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| trans-1,3-Dichloropropene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0846 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| Trichloroethene | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.0993 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| Trichlorofluoromethane | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.134 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| Vinyl chloride | A | ug/L | 0 | 0 | | 0 | 0 | 0 | 0.153 | 0.5 | 500 | 0% | 0 | 0 | 0% | U |
| 1,4-Dichlorobenzene-d4 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 0 | 0 | 0% | |
| Chlorobenzene-d5 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 0 | 0 | 0% | |
| Fluorobenzene | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 0 | 0 | 0% | |
| Xylenes, Total | M | ug/L | 2.13119 | 0.0852476 | | 0 | 0 | 0 | 0.0604 | 0.5 | 1500 | 0% | 0 | 0 | 0% | J |
| 1,2-Dichloroethane-d4 | S | ug/L | 295.27075 | 11.81083 | | 10 | 0 | 0 | 0.229 | 0.5 | 500 | 118% | 81 | 118 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|----------------------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971553 | B22010002-001 | VOC-8260-W-Q | SAMP | DA5975C\VG010:1/5/2022 | 4:00:32 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| Dibromofluoromethane | S | ug/L | 278.55532 | 11.1422128 | | 10 | 0 | 0 | 0.129 | 0.5 | 500 | 111% | 80 | 119 | 0% | |
| p-Bromofluorobenzene | S | ug/L | 264.11239 | 10.5644956 | | 10 | 0 | 0 | 0.149 | 0.5 | 500 | 106% | 85 | 114 | 0% | |
| Toluene-d8 | S | ug/L | 264.08962 | 10.5635848 | | 10 | 0 | 0 | 0.23 | 0.5 | 500 | 106% | 89 | 112 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|---------------|--------------|------------|------------------------|---------------|-------|-----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971554 | B22010002-001 | VOC-8260-W-Q | MS-DOD | DA5975C\VG010:1/5/2022 | 8:33:23 | 1 | R372966 | | 1E+07 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A | ug/L | 124.2913 | 4.971652 | | 5 | 0 | 0 | 0.101 | 0.5 | 500 | 99% | 78 | 124 | 0% | |
| 1,1,1-Trichloroethane | A | ug/L | 126.81306 | 5.0725224 | | 5 | 0 | 0 | 0.131 | 0.5 | 500 | 101% | 74 | 131 | 0% | |
| 1,1,2,2-Tetrachloroethane | A | ug/L | 130.0529 | 5.202116 | | 5 | 0 | 0 | 0.0872 | 0.5 | 500 | 104% | 71 | 121 | 0% | |
| 1,1,2-Trichloroethane | A | ug/L | 125.70778 | 5.0283112 | | 5 | 0 | 0 | 0.108 | 0.5 | 500 | 101% | 80 | 119 | 0% | |
| 1,1-Dichloroethane | A | ug/L | 131.63166 | 5.2652664 | | 5 | 0 | 0 | 0.135 | 0.5 | 500 | 105% | 77 | 125 | 0% | |
| 1,1-Dichloroethene | A | ug/L | 130.81807 | 5.2327228 | | 5 | 0 | 0 | 0.141 | 0.5 | 500 | 105% | 71 | 131 | 0% | |
| 1,1-Dichloropropene | A | ug/L | 118.88429 | 4.7553716 | | 5 | 0 | 0 | 0.083 | 0.5 | 500 | 95% | 79 | 125 | 0% | |
| 1,2,3-Trichloropropane | A | ug/L | 124.14169 | 4.9656676 | | 5 | 0 | 0 | 0.235 | 0.5 | 500 | 99% | 73 | 125 | 0% | |
| 1,2-Dibromoethane | A | ug/L | 124.69649 | 4.9878596 | | 5 | 0 | 0 | 0.0916 | 0.5 | 500 | 100% | 78 | 122 | 0% | |
| 1,2-Dichlorobenzene | A | ug/L | 127.18373 | 5.0873492 | | 5 | 0 | 0 | 0.0746 | 0.5 | 500 | 102% | 80 | 119 | 0% | |
| 1,2-Dichloroethane | A | ug/L | 123.53198 | 4.9412792 | | 5 | 0 | 0 | 0.116 | 0.5 | 500 | 99% | 73 | 128 | 0% | |
| 1,2-Dichloropropane | A | ug/L | 123.48815 | 4.939526 | | 5 | 0 | 0 | 0.0847 | 0.5 | 500 | 99% | 78 | 122 | 0% | |
| 1,3-Dichlorobenzene | A | ug/L | 128.44151 | 5.1376604 | | 5 | 0 | 0 | 0.0803 | 0.5 | 500 | 103% | 80 | 119 | 0% | |
| 1,3-Dichloropropane | A | ug/L | 122.44612 | 4.8978448 | | 5 | 0 | 0 | 0.0791 | 0.5 | 500 | 98% | 80 | 119 | 0% | |
| 1,4-Dichlorobenzene | A | ug/L | 127.49417 | 5.0997668 | | 5 | 0 | 0 | 0.0858 | 0.5 | 500 | 102% | 79 | 118 | 0% | |
| 2,2-Dichloropropane | A | ug/L | 124.6457 | 4.985828 | | 5 | 0 | 0 | 0.186 | 0.5 | 500 | 100% | 60 | 139 | 0% | |
| 2-Chlorotoluene | A | ug/L | 131.40376 | 5.2561504 | | 5 | 0 | 0 | 0.0876 | 0.5 | 500 | 105% | 79 | 122 | 0% | |
| 4-Chlorotoluene | A | ug/L | 131.94766 | 5.2779064 | | 5 | 0 | 0 | 0.0728 | 0.5 | 500 | 106% | 78 | 122 | 0% | |
| Benzene | A | ug/L | 129.18093 | 5.1672372 | | 5 | 0 | 0 | 0.0914 | 0.5 | 500 | 103% | 79 | 120 | 0% | |
| Bromobenzene | A | ug/L | 130.84998 | 5.2339992 | | 5 | 0 | 0 | 0.0831 | 0.5 | 500 | 105% | 80 | 120 | 0% | |
| Bromochloromethane | A | ug/L | 123.80263 | 4.9521052 | | 5 | 0 | 0 | 0.141 | 0.5 | 500 | 99% | 78 | 123 | 0% | |
| Bromodichloromethane | A | ug/L | 130.40783 | 5.2163132 | | 5 | 0 | 0 | 0.12 | 0.5 | 500 | 104% | 79 | 125 | 0% | |
| Bromoform | A | ug/L | 141.29554 | 5.6518216 | | 5 | 0.6619312 | 0 | 0.119 | 0.5 | 500 | 100% | 66 | 130 | 0% | |
| Bromomethane | A | ug/L | 104.79494 | 4.1917976 | | 5 | 0 | 0 | 0.253 | 0.5 | 500 | 84% | 53 | 141 | 0% | |
| Carbon tetrachloride | A | ug/L | 124.23425 | 4.96937 | | 5 | 0 | 0 | 0.143 | 0.5 | 500 | 99% | 72 | 136 | 0% | |
| Chlorobenzene | A | ug/L | 125.98193 | 5.0392772 | | 5 | 0 | 0 | 0.0914 | 0.5 | 500 | 101% | 82 | 118 | 0% | |
| Chlorodibromomethane | A | ug/L | 131.48391 | 5.2593564 | | 5 | 0.2318016 | 0 | 0.0841 | 0.5 | 500 | 101% | 74 | 126 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|--------------------------------|---------------|--------------|------------|------------------------|---------------|-------|-----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971554 | B22010002-001 | VOC-8260-W-Q | MS-DOD | DA5975C\VG010:1/5/2022 | 8:33:23 | 1 | R372966 | | 1E+07 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| Chloroethane | A | ug/L | 105.22062 | 4.2088248 | | 5 | 0 | 0 | 0.169 | 0.5 | 500 | 84% | 60 | 138 | 0% | |
| Chloroform | A | ug/L | 122.94551 | 4.9178204 | | 5 | 0 | 0 | 0.0789 | 0.5 | 500 | 98% | 79 | 124 | 0% | |
| Chloromethane | A | ug/L | 105.90169 | 4.2360676 | | 5 | 0 | 0 | 0.162 | 0.5 | 500 | 85% | 50 | 139 | 0% | |
| cis-1,2-Dichloroethene | A | ug/L | 130.07041 | 5.2028164 | | 5 | 0 | 0 | 0.108 | 0.5 | 500 | 104% | 78 | 123 | 0% | |
| cis-1,3-Dichloropropene | A | ug/L | 114.74869 | 4.5899476 | | 5 | 0 | 0 | 0.073 | 0.5 | 500 | 92% | 75 | 124 | 0% | |
| Dibromomethane | A | ug/L | 128.63758 | 5.1455032 | | 5 | 0 | 0 | 0.147 | 0.5 | 500 | 103% | 79 | 123 | 0% | |
| Dichlorodifluoromethane | A | ug/L | 110.02865 | 4.401146 | | 5 | 0 | 0 | 0.175 | 0.5 | 500 | 88% | 32 | 152 | 0% | |
| Ethylbenzene | A | ug/L | 126.9581 | 5.078324 | | 5 | 0 | 0 | 0.0836 | 0.5 | 500 | 102% | 79 | 121 | 0% | |
| m+p-Xylenes | A | ug/L | 257.70968 | 10.3083872 | | 10 | 0 | 0 | 0.15 | 0.5 | 1000 | 103% | 80 | 121 | 0% | |
| Methyl ethyl ketone | A | ug/L | 1221.12605 | 48.845042 | | 50 | 0 | 0 | 1.77 | 10 | 5000 | 98% | 56 | 143 | 0% | |
| Methyl tert-butyl ether (MTBE) | A | ug/L | 135.78671 | 5.4314684 | | 5 | 0 | 0 | 0.101 | 0.5 | 500 | 109% | 71 | 124 | 0% | |
| Methylene chloride | A | ug/L | 120.44673 | 4.8178692 | | 5 | 0 | 0 | 0.338 | 0.5 | 500 | 96% | 74 | 124 | 0% | |
| o-Xylene | A | ug/L | 129.95296 | 5.1981184 | | 5 | 0.0852476 | 0 | 0.0604 | 0.5 | 500 | 102% | 78 | 122 | 0% | |
| Styrene | A | ug/L | 133.36669 | 5.3346676 | | 5 | 0 | 0 | 0.067 | 0.5 | 500 | 107% | 78 | 123 | 0% | |
| Tetrachloroethene | A | ug/L | 124.83053 | 4.9932212 | | 5 | 0 | 0 | 0.0671 | 0.5 | 500 | 100% | 74 | 129 | 0% | |
| Toluene | A | ug/L | 130.26584 | 5.2106336 | | 5 | 0 | 0 | 0.0679 | 0.5 | 500 | 104% | 80 | 121 | 0% | |
| trans-1,2-Dichloroethene | A | ug/L | 128.76558 | 5.1506232 | | 5 | 0 | 0 | 0.125 | 0.5 | 500 | 103% | 75 | 124 | 0% | |
| trans-1,3-Dichloropropene | A | ug/L | 128.12439 | 5.1249756 | | 5 | 0 | 0 | 0.0846 | 0.5 | 500 | 102% | 73 | 127 | 0% | |
| Trichloroethene | A | ug/L | 127.07003 | 5.0828012 | | 5 | 0 | 0 | 0.0993 | 0.5 | 500 | 102% | 79 | 123 | 0% | |
| Trichlorofluoromethane | A | ug/L | 120.46314 | 4.8185256 | | 5 | 0 | 0 | 0.134 | 0.5 | 500 | 96% | 65 | 141 | 0% | |
| Vinyl chloride | A | ug/L | 116.32383 | 4.6529532 | | 5 | 0 | 0 | 0.153 | 0.5 | 500 | 93% | 58 | 137 | 0% | |
| 1,4-Dichlorobenzene-d4 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 0 | 0 | 0% | |
| Chlorobenzene-d5 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 0 | 0 | 0% | |
| Fluorobenzene | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 0 | 0 | 0% | |
| Xylenes, Total | M | ug/L | 387.66264 | 15.5065056 | | 15 | 0.0852476 | 0 | 0.0604 | 0.5 | 1500 | 103% | 79 | 121 | 0% | |
| 1,2-Dichloroethane-d4 | S | ug/L | 281.72264 | 11.2689056 | | 10 | 0 | 0 | 0.229 | 0.5 | 500 | 113% | 81 | 118 | 0% | |
| Dibromofluoromethane | S | ug/L | 274.31186 | 10.9724744 | | 10 | 0 | 0 | 0.129 | 0.5 | 500 | 110% | 80 | 119 | 0% | |
| p-Bromofluorobenzene | S | ug/L | 262.94255 | 10.517702 | | 10 | 0 | 0 | 0.149 | 0.5 | 500 | 105% | 85 | 114 | 0% | |
| Toluene-d8 | S | ug/L | 279.18451 | 11.1673804 | | 10 | 0 | 0 | 0.23 | 0.5 | 500 | 112% | 89 | 112 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|----------|---------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971555 | B22010002-001 | VOC-8260-W-Q | MSD-DOD | DA5975C\VG010:1/5/2022 | 9:00:38 | 1 | R372966 | | 1E+07 | 1E+07 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|---------------|--------------|------------|------------------------|---------------|-------|-----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971555 | B22010002-001 | VOC-8260-W-Q | MSD-DOD | DA5975C\VG010:1/5/2022 | 9:00:38 | 1 | R372966 | | 1E+07 | 1E+07 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A | ug/L | 129.55639 | 5.1822556 | | 5 | 0 | 4.971652 | 0.101 | 0.5 | 500 | 104% | 78 | 124 | 4% | |
| 1,1,1-Trichloroethane | A | ug/L | 136.27134 | 5.4508536 | | 5 | 0 | 5.0725224 | 0.131 | 0.5 | 500 | 109% | 74 | 131 | 7% | |
| 1,1,2,2-Tetrachloroethane | A | ug/L | 138.83661 | 5.5534644 | | 5 | 0 | 5.202116 | 0.0872 | 0.5 | 500 | 111% | 71 | 121 | 7% | |
| 1,1,2-Trichloroethane | A | ug/L | 131.14249 | 5.2456996 | | 5 | 0 | 5.0283112 | 0.108 | 0.5 | 500 | 105% | 80 | 119 | 4% | |
| 1,1-Dichloroethane | A | ug/L | 142.83081 | 5.7132324 | | 5 | 0 | 5.2652664 | 0.135 | 0.5 | 500 | 114% | 77 | 125 | 8% | |
| 1,1-Dichloroethene | A | ug/L | 140.22157 | 5.6088628 | | 5 | 0 | 5.2327228 | 0.141 | 0.5 | 500 | 112% | 71 | 131 | 7% | |
| 1,1-Dichloropropene | A | ug/L | 129.15526 | 5.1662104 | | 5 | 0 | 4.7553716 | 0.083 | 0.5 | 500 | 103% | 79 | 125 | 8% | |
| 1,2,3-Trichloropropane | A | ug/L | 139.49707 | 5.5798828 | | 5 | 0 | 4.9656676 | 0.235 | 0.5 | 500 | 112% | 73 | 125 | 12% | |
| 1,2-Dibromoethane | A | ug/L | 137.04445 | 5.481778 | | 5 | 0 | 4.9878596 | 0.0916 | 0.5 | 500 | 110% | 78 | 122 | 9% | |
| 1,2-Dichlorobenzene | A | ug/L | 136.84112 | 5.4736448 | | 5 | 0 | 5.0873492 | 0.0746 | 0.5 | 500 | 109% | 80 | 119 | 7% | |
| 1,2-Dichloroethane | A | ug/L | 134.14629 | 5.3658516 | | 5 | 0 | 4.9412792 | 0.116 | 0.5 | 500 | 107% | 73 | 128 | 8% | |
| 1,2-Dichloropropane | A | ug/L | 133.1065 | 5.32426 | | 5 | 0 | 4.939526 | 0.0847 | 0.5 | 500 | 106% | 78 | 122 | 7% | |
| 1,3-Dichlorobenzene | A | ug/L | 136.27909 | 5.4511636 | | 5 | 0 | 5.1376604 | 0.0803 | 0.5 | 500 | 109% | 80 | 119 | 6% | |
| 1,3-Dichloropropane | A | ug/L | 132.2893 | 5.291572 | | 5 | 0 | 4.8978448 | 0.0791 | 0.5 | 500 | 106% | 80 | 119 | 8% | |
| 1,4-Dichlorobenzene | A | ug/L | 134.30285 | 5.372114 | | 5 | 0 | 5.0997668 | 0.0858 | 0.5 | 500 | 107% | 79 | 118 | 5% | |
| 2,2-Dichloropropane | A | ug/L | 132.48722 | 5.2994888 | | 5 | 0 | 4.985828 | 0.186 | 0.5 | 500 | 106% | 60 | 139 | 6% | |
| 2-Chlorotoluene | A | ug/L | 140.15256 | 5.6061024 | | 5 | 0 | 5.2561504 | 0.0876 | 0.5 | 500 | 112% | 79 | 122 | 6% | |
| 4-Chlorotoluene | A | ug/L | 140.68991 | 5.6275964 | | 5 | 0 | 5.2779064 | 0.0728 | 0.5 | 500 | 113% | 78 | 122 | 6% | |
| Benzene | A | ug/L | 136.34074 | 5.4536296 | | 5 | 0 | 5.1672372 | 0.0914 | 0.5 | 500 | 109% | 79 | 120 | 5% | |
| Bromobenzene | A | ug/L | 135.73709 | 5.4294836 | | 5 | 0 | 5.2339992 | 0.0831 | 0.5 | 500 | 109% | 80 | 120 | 4% | |
| Bromochloromethane | A | ug/L | 133.76756 | 5.3507024 | | 5 | 0 | 4.9521052 | 0.141 | 0.5 | 500 | 107% | 78 | 123 | 8% | |
| Bromodichloromethane | A | ug/L | 138.93129 | 5.5572516 | | 5 | 0 | 5.2163132 | 0.12 | 0.5 | 500 | 111% | 79 | 125 | 6% | |
| Bromoform | A | ug/L | 159.40334 | 6.3761336 | | 5 | 0.6619312 | 5.6518216 | 0.119 | 0.5 | 500 | 114% | 66 | 130 | 12% | |
| Bromomethane | A | ug/L | 119.28739 | 4.7714956 | | 5 | 0 | 4.1917976 | 0.253 | 0.5 | 500 | 95% | 53 | 141 | 13% | |
| Carbon tetrachloride | A | ug/L | 132.5551 | 5.302204 | | 5 | 0 | 4.96937 | 0.143 | 0.5 | 500 | 106% | 72 | 136 | 6% | |
| Chlorobenzene | A | ug/L | 134.83984 | 5.3935936 | | 5 | 0 | 5.0392772 | 0.0914 | 0.5 | 500 | 108% | 82 | 118 | 7% | |
| Chlorodibromomethane | A | ug/L | 142.81647 | 5.7126588 | | 5 | 0.2318016 | 5.2593564 | 0.0841 | 0.5 | 500 | 110% | 74 | 126 | 8% | |
| Chloroethane | A | ug/L | 113.24726 | 4.5298904 | | 5 | 0 | 4.2088248 | 0.169 | 0.5 | 500 | 91% | 60 | 138 | 7% | |
| Chloroform | A | ug/L | 128.63808 | 5.1455232 | | 5 | 0 | 4.9178204 | 0.0789 | 0.5 | 500 | 103% | 79 | 124 | 5% | |
| Chloromethane | A | ug/L | 115.97135 | 4.638854 | | 5 | 0 | 4.2360676 | 0.162 | 0.5 | 500 | 93% | 50 | 139 | 9% | |
| cis-1,2-Dichloroethene | A | ug/L | 137.91242 | 5.5164968 | | 5 | 0 | 5.2028164 | 0.108 | 0.5 | 500 | 110% | 78 | 123 | 6% | |
| cis-1,3-Dichloropropene | A | ug/L | 125.53217 | 5.0212868 | | 5 | 0 | 4.5899476 | 0.073 | 0.5 | 500 | 100% | 75 | 124 | 9% | |
| Dibromomethane | A | ug/L | 131.63685 | 5.265474 | | 5 | 0 | 5.1455032 | 0.147 | 0.5 | 500 | 105% | 79 | 123 | 2% | |
| Dichlorodifluoromethane | A | ug/L | 117.14005 | 4.685602 | | 5 | 0 | 4.401146 | 0.175 | 0.5 | 500 | 94% | 32 | 152 | 6% | |
| Ethylbenzene | A | ug/L | 133.66902 | 5.3467608 | | 5 | 0 | 5.078324 | 0.0836 | 0.5 | 500 | 107% | 79 | 121 | 5% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|--------------------------------|---------------|--------------|------------|------------------------|---------------|-------|-----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971555 | B22010002-001 | VOC-8260-W-Q | MSD-DOD | DA5975C\VG010:1/5/2022 | 9:00:38 | 1 | R372966 | | 1E+07 | 1E+07 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| m+p-Xylenes | A | ug/L | 269.98414 | 10.7993656 | | 10 | 0 | 10.308387 | 0.15 | 0.5 | 1000 | 108% | 80 | 121 | 5% | |
| Methyl ethyl ketone | A | ug/L | 1322.90752 | 52.9163008 | | 50 | 0 | 48.845042 | 1.77 | 10 | 5000 | 106% | 56 | 143 | 8% | |
| Methyl tert-butyl ether (MTBE) | A | ug/L | 143.34393 | 5.7337572 | | 5 | 0 | 5.4314684 | 0.101 | 0.5 | 500 | 115% | 71 | 124 | 5% | |
| Methylene chloride | A | ug/L | 126.60809 | 5.0643236 | | 5 | 0 | 4.8178692 | 0.338 | 0.5 | 500 | 101% | 74 | 124 | 5% | |
| o-Xylene | A | ug/L | 137.75032 | 5.5100128 | | 5 | 0.0852476 | 5.1981184 | 0.0604 | 0.5 | 500 | 108% | 78 | 122 | 6% | |
| Styrene | A | ug/L | 137.60624 | 5.5042496 | | 5 | 0 | 5.3346676 | 0.067 | 0.5 | 500 | 110% | 78 | 123 | 3% | |
| Tetrachloroethene | A | ug/L | 131.87767 | 5.2751068 | | 5 | 0 | 4.9932212 | 0.0671 | 0.5 | 500 | 106% | 74 | 129 | 5% | |
| Toluene | A | ug/L | 136.05295 | 5.442118 | | 5 | 0 | 5.2106336 | 0.0679 | 0.5 | 500 | 109% | 80 | 121 | 4% | |
| trans-1,2-Dichloroethene | A | ug/L | 140.14648 | 5.6058592 | | 5 | 0 | 5.1506232 | 0.125 | 0.5 | 500 | 112% | 75 | 124 | 8% | |
| trans-1,3-Dichloropropene | A | ug/L | 137.99611 | 5.5198444 | | 5 | 0 | 5.1249756 | 0.0846 | 0.5 | 500 | 110% | 73 | 127 | 7% | |
| Trichloroethene | A | ug/L | 131.90292 | 5.2761168 | | 5 | 0 | 5.0828012 | 0.0993 | 0.5 | 500 | 106% | 79 | 123 | 4% | |
| Trichlorofluoromethane | A | ug/L | 121.42559 | 4.8570236 | | 5 | 0 | 4.8185256 | 0.134 | 0.5 | 500 | 97% | 65 | 141 | 1% | |
| Vinyl chloride | A | ug/L | 127.00993 | 5.0803972 | | 5 | 0 | 4.6529532 | 0.153 | 0.5 | 500 | 102% | 58 | 137 | 9% | |
| 1,4-Dichlorobenzene-d4 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 0 | 0 | 0% | |
| Chlorobenzene-d5 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 0 | 0 | 0% | |
| Fluorobenzene | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 0 | 0 | 0% | |
| Xylenes, Total | M | ug/L | 407.73446 | 16.3093784 | | 15 | 0.0852476 | 15.506506 | 0.0604 | 0.5 | 1500 | 108% | 79 | 121 | 5% | |
| 1,2-Dichloroethane-d4 | S | ug/L | 283.13107 | 11.3252428 | | 10 | 0 | 0 | 0.229 | 0.5 | 500 | 113% | 81 | 118 | 0% | |
| Dibromofluoromethane | S | ug/L | 273.11605 | 10.924642 | | 10 | 0 | 0 | 0.129 | 0.5 | 500 | 109% | 80 | 119 | 0% | |
| p-Bromofluorobenzene | S | ug/L | 269.28041 | 10.7712164 | | 10 | 0 | 0 | 0.149 | 0.5 | 500 | 108% | 85 | 114 | 0% | |
| Toluene-d8 | S | ug/L | 276.19485 | 11.047794 | | 10 | 0 | 0 | 0.23 | 0.5 | 500 | 110% | 89 | 112 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|--------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971556 | CCV010522_CI | VOC-8260-W-Q | CCV | DA5975C\VG010:1/5/2022 | 9:55:17 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A | ug/L | 118.49712 | 4.7398848 | | 5 | 0 | 0 | 0.101 | 0.5 | 500 | 95% | 50 | 150 | 0% | |
| 1,1,1-Trichloroethane | A | ug/L | 121.22736 | 4.8490944 | | 5 | 0 | 0 | 0.131 | 0.5 | 500 | 97% | 50 | 150 | 0% | |
| 1,1,2,2-Tetrachloroethane | A | ug/L | 119.79308 | 4.7917232 | | 5 | 0 | 0 | 0.0872 | 0.5 | 500 | 96% | 50 | 150 | 0% | |
| 1,1,2-Trichloroethane | A | ug/L | 115.36074 | 4.6144296 | | 5 | 0 | 0 | 0.108 | 0.5 | 500 | 92% | 50 | 150 | 0% | |
| 1,1-Dichloroethane | A | ug/L | 122.22572 | 4.8890288 | | 5 | 0 | 0 | 0.135 | 0.5 | 500 | 98% | 50 | 150 | 0% | |
| 1,1-Dichloroethene | A | ug/L | 120.16154 | 4.8064616 | | 5 | 0 | 0 | 0.141 | 0.5 | 500 | 96% | 50 | 150 | 0% | |
| 1,1-Dichloropropene | A | ug/L | 121.57324 | 4.8629296 | | 5 | 0 | 0 | 0.083 | 0.5 | 500 | 97% | 50 | 150 | 0% | |
| 1,2,3-Trichloropropane | A | ug/L | 110.61728 | 4.4246912 | | 5 | 0 | 0 | 0.235 | 0.5 | 500 | 88% | 50 | 150 | 0% | |
| 1,2-Dibromoethane | A | ug/L | 114.75493 | 4.5901972 | | 5 | 0 | 0 | 0.0916 | 0.5 | 500 | 92% | 50 | 150 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|--------------------------------|--------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971556 | CCV010522_CI | VOC-8260-W-Q | CCV | DA5975C\VG010:1/5/2022 | 9:55:17 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| 1,2-Dichlorobenzene | A | ug/L | 118.57342 | 4.7429368 | | 5 | 0 | 0 | 0.0746 | 0.5 | 500 | 95% | 50 | 150 | 0% | |
| 1,2-Dichloroethane | A | ug/L | 119.94088 | 4.7976352 | | 5 | 0 | 0 | 0.116 | 0.5 | 500 | 96% | 50 | 150 | 0% | |
| 1,2-Dichloropropane | A | ug/L | 115.63029 | 4.6252116 | | 5 | 0 | 0 | 0.0847 | 0.5 | 500 | 93% | 50 | 150 | 0% | |
| 1,3-Dichlorobenzene | A | ug/L | 121.04602 | 4.8418408 | | 5 | 0 | 0 | 0.0803 | 0.5 | 500 | 97% | 50 | 150 | 0% | |
| 1,3-Dichloropropane | A | ug/L | 118.36911 | 4.7347644 | | 5 | 0 | 0 | 0.0791 | 0.5 | 500 | 95% | 50 | 150 | 0% | |
| 1,4-Dichlorobenzene | A | ug/L | 117.19516 | 4.6878064 | | 5 | 0 | 0 | 0.0858 | 0.5 | 500 | 94% | 50 | 150 | 0% | |
| 2,2-Dichloropropane | A | ug/L | 119.01241 | 4.7604964 | | 5 | 0 | 0 | 0.186 | 0.5 | 500 | 95% | 50 | 150 | 0% | |
| 2-Chlorotoluene | A | ug/L | 125.61814 | 5.0247256 | | 5 | 0 | 0 | 0.0876 | 0.5 | 500 | 100% | 50 | 150 | 0% | |
| 4-Chlorotoluene | A | ug/L | 125.36003 | 5.0144012 | | 5 | 0 | 0 | 0.0728 | 0.5 | 500 | 100% | 50 | 150 | 0% | |
| Benzene | A | ug/L | 122.53031 | 4.9012124 | | 5 | 0 | 0 | 0.0914 | 0.5 | 500 | 98% | 50 | 150 | 0% | |
| Bromobenzene | A | ug/L | 124.30294 | 4.9721176 | | 5 | 0 | 0 | 0.0831 | 0.5 | 500 | 99% | 50 | 150 | 0% | |
| Bromochloromethane | A | ug/L | 120.31319 | 4.8125276 | | 5 | 0 | 0 | 0.141 | 0.5 | 500 | 96% | 50 | 150 | 0% | |
| Bromodichloromethane | A | ug/L | 119.0304 | 4.761216 | | 5 | 0 | 0 | 0.12 | 0.5 | 500 | 95% | 50 | 150 | 0% | |
| Bromoform | A | ug/L | 121.44048 | 4.8576192 | | 5 | 0 | 0 | 0.119 | 0.5 | 500 | 97% | 50 | 150 | 0% | |
| Bromomethane | A | ug/L | 123.70271 | 4.9481084 | | 5 | 0 | 0 | 0.253 | 0.5 | 500 | 99% | 50 | 150 | 0% | |
| Carbon tetrachloride | A | ug/L | 121.82703 | 4.8730812 | | 5 | 0 | 0 | 0.143 | 0.5 | 500 | 97% | 50 | 150 | 0% | |
| Chlorobenzene | A | ug/L | 120.60357 | 4.8241428 | | 5 | 0 | 0 | 0.0914 | 0.5 | 500 | 96% | 50 | 150 | 0% | |
| Chlorodibromomethane | A | ug/L | 118.11044 | 4.7244176 | | 5 | 0 | 0 | 0.0841 | 0.5 | 500 | 94% | 50 | 150 | 0% | |
| Chloroethane | A | ug/L | 110.53218 | 4.4212872 | | 5 | 0 | 0 | 0.169 | 0.5 | 500 | 88% | 50 | 150 | 0% | |
| Chloroform | A | ug/L | 116.26028 | 4.6504112 | | 5 | 0 | 0 | 0.0789 | 0.5 | 500 | 93% | 50 | 150 | 0% | |
| Chloromethane | A | ug/L | 117.04699 | 4.6818796 | | 5 | 0 | 0 | 0.162 | 0.5 | 500 | 94% | 50 | 150 | 0% | |
| cis-1,2-Dichloroethene | A | ug/L | 121.6867 | 4.867468 | | 5 | 0 | 0 | 0.108 | 0.5 | 500 | 97% | 50 | 150 | 0% | |
| cis-1,3-Dichloropropene | A | ug/L | 113.32001 | 4.5328004 | | 5 | 0 | 0 | 0.073 | 0.5 | 500 | 91% | 50 | 150 | 0% | |
| Dibromomethane | A | ug/L | 118.13357 | 4.7253428 | | 5 | 0 | 0 | 0.147 | 0.5 | 500 | 95% | 50 | 150 | 0% | |
| Dichlorodifluoromethane | A | ug/L | 120.80768 | 4.8323072 | | 5 | 0 | 0 | 0.175 | 0.5 | 500 | 97% | 50 | 150 | 0% | |
| Ethylbenzene | A | ug/L | 120.81542 | 4.8326168 | | 5 | 0 | 0 | 0.0836 | 0.5 | 500 | 97% | 50 | 150 | 0% | |
| m+p-Xylenes | A | ug/L | 251.01571 | 10.0406284 | | 10 | 0 | 0 | 0.15 | 0.5 | 1000 | 100% | 50 | 150 | 0% | |
| Methyl ethyl ketone | A | ug/L | 1129.33406 | 45.1733624 | | 50 | 0 | 0 | 1.77 | 10 | 5000 | 90% | 50 | 150 | 0% | |
| Methyl tert-butyl ether (MTBE) | A | ug/L | 117.72622 | 4.7090488 | | 5 | 0 | 0 | 0.101 | 0.5 | 500 | 94% | 50 | 150 | 0% | |
| Methylene chloride | A | ug/L | 112.74658 | 4.5098632 | | 5 | 0 | 0 | 0.338 | 0.5 | 500 | 90% | 50 | 150 | 0% | |
| o-Xylene | A | ug/L | 123.05663 | 4.9222652 | | 5 | 0 | 0 | 0.0604 | 0.5 | 500 | 98% | 50 | 150 | 0% | |
| Styrene | A | ug/L | 126.92772 | 5.0771088 | | 5 | 0 | 0 | 0.067 | 0.5 | 500 | 102% | 50 | 150 | 0% | |
| Tetrachloroethene | A | ug/L | 119.13237 | 4.7652948 | | 5 | 0 | 0 | 0.0671 | 0.5 | 500 | 95% | 50 | 150 | 0% | |
| Toluene | A | ug/L | 121.81649 | 4.8726596 | | 5 | 0 | 0 | 0.0679 | 0.5 | 500 | 97% | 50 | 150 | 0% | |
| trans-1,2-Dichloroethene | A | ug/L | 122.59387 | 4.9037548 | | 5 | 0 | 0 | 0.125 | 0.5 | 500 | 98% | 50 | 150 | 0% | |

| Seq No | Lab ID | Test Code | Sample Typ | File ID | Analysis Date | DF | Batch ID | Prep Date | SPKref | RPDref | pmoist | | | | | |
|---------------------------|--------------|--------------|------------|------------------------|---------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14971556 | CCV010522_CI | VOC-8260-W-Q | CCV | DA5975C\VG010:1/5/2022 | 9:55:17 | 1 | R372966 | | 0 | 0 | | | | | | |
| Analyte | T | Units | RAW | Final | Text | Spike | SPKref | RPDref | MDL | PQL | UQL | %REC | LOW | HIGH | %RPD | Q |
| trans-1,3-Dichloropropene | A | ug/L | 119.58825 | 4.78353 | | 5 | 0 | 0 | 0.0846 | 0.5 | 500 | 96% | 50 | 150 | 0% | |
| Trichloroethene | A | ug/L | 121.06211 | 4.8424844 | | 5 | 0 | 0 | 0.0993 | 0.5 | 500 | 97% | 50 | 150 | 0% | |
| Trichlorofluoromethane | A | ug/L | 122.98084 | 4.9192336 | | 5 | 0 | 0 | 0.134 | 0.5 | 500 | 98% | 50 | 150 | 0% | |
| Vinyl chloride | A | ug/L | 119.38078 | 4.7752312 | | 5 | 0 | 0 | 0.153 | 0.5 | 500 | 96% | 50 | 150 | 0% | |
| 1,4-Dichlorobenzene-d4 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 0 | 0 | 0% | |
| Chlorobenzene-d5 | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 0 | 0 | 0% | |
| Fluorobenzene | I | ug/L | 250 | 10 | | 0 | 0 | 0 | 0 | 0 | 500 | 0% | 0 | 0 | 0% | |
| Xylenes, Total | M | ug/L | 374.07234 | 14.9628936 | | 15 | 0 | 0 | 0.0604 | 0.5 | 1500 | 100% | 50 | 150 | 0% | |
| 1,2-Dichloroethane-d4 | S | ug/L | 278.44117 | 11.1376468 | | 10 | 0 | 0 | 0.229 | 0.5 | 500 | 111% | 50 | 150 | 0% | |
| Dibromofluoromethane | S | ug/L | 270.98246 | 10.8392984 | | 10 | 0 | 0 | 0.129 | 0.5 | 500 | 108% | 50 | 150 | 0% | |
| p-Bromofluorobenzene | S | ug/L | 266.37534 | 10.6550136 | | 10 | 0 | 0 | 0.149 | 0.5 | 500 | 107% | 50 | 150 | 0% | |
| Toluene-d8 | S | ug/L | 275.15042 | 11.0060168 | | 10 | 0 | 0 | 0.23 | 0.5 | 500 | 110% | 50 | 150 | 0% | |

DATAFILE HEADERS FROM C:\MSDCHEM\1\DATA\VG010522

Data file Name : C:\MSDCHEM\1\DATA\VG010522\05JAN01.D
Sample Name : BLK
Operator : MSC
Date injected : 5 Jan 2022 9:22 am
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 1

Data file Name : C:\MSDCHEM\1\DATA\VG010522\05JAN02.D
Sample Name : BFB010522_
Operator : MSC
Date injected : 5 Jan 2022 9:49 am
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 2

Data file Name : C:\MSDCHEM\1\DATA\VG010522\05JAN03.D
Sample Name : CCV010522_
Operator : MSC
Date injected : 5 Jan 2022 10:28 am
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 3

Data file Name : C:\MSDCHEM\1\DATA\VG010522\05JAN04.D
Sample Name : LCS010522_
Operator : MSC
Date injected : 5 Jan 2022 11:27 am
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 4

Data file Name : C:\MSDCHEM\1\DATA\VG010522\05JAN05.D

Sample Name : BLK
Operator : MSC
Date injected : 5 Jan 2022 11:54 am
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 5

Data file Name : C:\MSDCHEM\1\DATA\VG010522\05JAN06.D
Sample Name : MBLK010522_
Operator : MSC
Date injected : 5 Jan 2022 12:21 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 6

Data file Name : C:\MSDCHEM\1\DATA\VG010522\05JAN07.D
Sample Name : B22010002-004A
Operator : MSC
Date injected : 5 Jan 2022 12:49 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 7

Data file Name : C:\MSDCHEM\1\DATA\VG010522\05JAN08.D
Sample Name : B22010096-002A
Operator : MSC
Date injected : 5 Jan 2022 1:16 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.839
End Time : 16.498
Vial Number : 8

Data file Name : C:\MSDCHEM\1\DATA\VG010522\05JAN09.D
Sample Name : B22010120-002A
Operator : MSC
Date injected : 5 Jan 2022 1:43 pm

Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 9

Data file Name : C:\MSDCHEM\1\DATA\VG010522\05JAN10.D
Sample Name : B22010134-002A
Operator : MSC
Date injected : 5 Jan 2022 2:11 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 10

Data file Name : C:\MSDCHEM\1\DATA\VG010522\05JAN11.D
Sample Name : B22010141-002A
Operator : MSC
Date injected : 5 Jan 2022 2:38 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 11

Data file Name : C:\MSDCHEM\1\DATA\VG010522\05JAN12.D
Sample Name : B22010142-002A
Operator : MSC
Date injected : 5 Jan 2022 3:05 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 12

Data file Name : C:\MSDCHEM\1\DATA\VG010522\05JAN13.D
Sample Name : B22010143-002A
Operator : MSC
Date injected : 5 Jan 2022 3:33 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616

Start Time : 0.840
End Time : 16.498
Vial Number : 13

Data file Name : C:\MSDCHEM\1\DATA\VG010522\05JAN14.D
Sample Name : B22010002-001F
Operator : MSC
Date injected : 5 Jan 2022 4:00 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 14

Data file Name : C:\MSDCHEM\1\DATA\VG010522\05JAN15.D
Sample Name : B22010002-002F
Operator : MSC
Date injected : 5 Jan 2022 4:27 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.839
End Time : 16.498
Vial Number : 15

Data file Name : C:\MSDCHEM\1\DATA\VG010522\05JAN16.D
Sample Name : B22010002-003C
Operator : MSC
Date injected : 5 Jan 2022 4:55 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 16

Data file Name : C:\MSDCHEM\1\DATA\VG010522\05JAN17.D
Sample Name : B22010096-001F
Operator : MSC
Date injected : 5 Jan 2022 5:22 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 17

Data file Name : C:\MSDCHEM\1\DATA\VG010522\05JAN18.D
Sample Name : B22010120-001F
Operator : MSC
Date injected : 5 Jan 2022 5:49 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 18

Data file Name : C:\MSDCHEM\1\DATA\VG010522\05JAN19.D
Sample Name : B22010134-001F
Operator : MSC
Date injected : 5 Jan 2022 6:16 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.839
End Time : 16.498
Vial Number : 19

Data file Name : C:\MSDCHEM\1\DATA\VG010522\05JAN20.D
Sample Name : B22010141-001F
Operator : MSC
Date injected : 5 Jan 2022 6:44 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.839
End Time : 16.498
Vial Number : 20

Data file Name : C:\MSDCHEM\1\DATA\VG010522\05JAN21.D
Sample Name : B22010142-001F
Operator : MSC
Date injected : 5 Jan 2022 7:11 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 21

Data file Name : C:\MSDCHEM\1\DATA\VG010522\05JAN22.D

Sample Name : B22010143-001F
Operator : MSC
Date injected : 5 Jan 2022 7:38 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 22

Data file Name : C:\MSDCHEM\1\DATA\VG010522\05JAN23.D
Sample Name : BLK
Operator : MSC
Date injected : 5 Jan 2022 8:06 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 23

Data file Name : C:\MSDCHEM\1\DATA\VG010522\05JAN24.D
Sample Name : B22010002-001FMS
Operator : MSC
Date injected : 5 Jan 2022 8:33 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 24

Data file Name : C:\MSDCHEM\1\DATA\VG010522\05JAN25.D
Sample Name : B22010002-001FMSD
Operator : MSC
Date injected : 5 Jan 2022 9:00 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 25

Data file Name : C:\MSDCHEM\1\DATA\VG010522\05JAN26.D
Sample Name : BLK
Operator : MSC
Date injected : 5 Jan 2022 9:27 pm

Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 26



Data file Name : C:\MSDCHEM\1\DATA\VG010522\05JAN27.D
Sample Name : CCV010522_Closing
Operator : MSC
Date injected : 5 Jan 2022 9:55 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 27

Data file Name : C:\MSDCHEM\1\DATA\VG010522\05JAN28.D
Sample Name : BLK
Operator : MSC
Date injected : 5 Jan 2022 10:22 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.839
End Time : 16.498
Vial Number : 28

Data file Name : C:\MSDCHEM\1\DATA\VG010522\05JAN29.D
Sample Name : BLK
Operator : MSC
Date injected : 5 Jan 2022 10:49 pm
Instrument : VOA5975C
Method used : 5975CACQF
No of spectra : 5616
Start Time : 0.840
End Time : 16.498
Vial Number : 29

Tune Evaluation Report

Data Path: D:\Org\Data\VOA5975C\VG010522\05JAN02.D
 Acq on: 1/5/2022 9:49:06 AM
 Operator: MSC
 Sample: BFB010522_
 Inst Name: VOA5975C
 ALS Vial: 2
 Method: \\MASSHUNTER\Org\Data\Methods\BFBapex.m



| Target Mass | Rel. To Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|-----------|
| 50 | 95 | 15 | 40 | 20.8 | 51832 | Pass |
| 75 | 95 | 30 | 60 | 48.4 | 120952 | Pass |
| 95 | 95 | 100 | 100 | 100.0 | 249664 | Pass |
| 96 | 95 | 5 | 9 | 6.4 | 15975 | Pass |
| 173 | 174 | 0 | 2 | 1.6 | 3650 | Pass |
| 174 | 95 | 50 | 100 | 92.0 | 229696 | Pass |
| 175 | 174 | 5 | 9 | 7.2 | 16424 | Pass |
| 176 | 174 | 95 | 101 | 96.9 | 222464 | Pass |
| 177 | 176 | 5 | 9 | 7.1 | 15712 | Pass |

Continuing Calibration Report

Batch Name D:\Org\Data\VOA5975C\VG010522\QuantResults\VG010522_8260B.batch.bin
Method File \\MASSHUNTER\Org\Data\Methods\Quant\VOA5975C\VOA5975C_010422_CAL\VOA5975C_8260B_SHT_DoD_L4_010422.m
Daily CC D:\Org\Data\VOA5975C\VG01052205JAN03.D

| Level name | Injection Time | Calibration Files |
|------------|----------------------|--|
| 1 | 1/4/2022 3:33:04 PM | D:\Org\Data\VOA5975C\VG010422\04JAN10.D |
| 2 | 1/4/2022 4:00:35 PM | D:\Org\Data\VOA5975C\VG010422\04JAN11.D |
| 3 | 1/4/2022 4:28:05 PM | D:\Org\Data\VOA5975C\VG010422\04JAN12.D |
| 4 | 1/4/2022 4:55:32 PM | D:\Org\Data\VOA5975C\VG010422\04JAN13.D |
| 5 | 1/4/2022 5:50:25 PM | D:\Org\Data\VOA5975C\VG010422\04JAN15.D |
| 6 | 1/4/2022 6:45:10 PM | D:\Org\Data\VOA5975C\VG010422\04JAN17.D |
| 7 | 1/4/2022 7:39:45 PM | D:\Org\Data\VOA5975C\VG010422\04JAN19.D |
| 8 | 1/4/2022 8:34:31 PM | D:\Org\Data\VOA5975C\VG010422\04JAN21.D |
| CC | 1/5/2022 10:28:43 AM | D:\Org\Data\VOA5975C\VG010522\05JAN03.D <===== |

| ISTD Compound: | Avg Resp | Mid Resp | CC Resp | Area% | A/M |
|------------------------|----------|----------|---------|-------|-----|
| Fluorobenzene | 805964 | 778120 | 758322 | 97.46 | M |
| Chlorobenzene-d5 | 305684 | 300356 | 289518 | 96.39 | M |
| 1,4-Dichlorobenzene-d4 | 252451 | 248636 | 242905 | 97.70 | M |

| Target Compound | AvgRF/R2 | CC RF | Exp. Conc | Calc. Conc | %Dev | Area% | Curve Fit |
|--------------------------------|----------|----------|-----------|------------|--------|--------|-----------|
| -----ISTD----- | | | | | | | |
| Dichlorodifluoromethane | 0.3276 | 0.3188 | 125.00 | 121.64 | 2.69 | 87.63 | Avg RF |
| Chloromethane | 0.3976 | 0.3861 | 125.00 | 121.37 | 2.90 | 91.15 | Avg RF |
| Vinyl chloride | 0.3578 | 0.3552 | 125.00 | 124.08 | 0.73 | 90.77 | Avg RF |
| Bromomethane | 0.1600 | 0.1673 | 125.00 | 130.74 | -4.59 | 97.37 | Avg RF |
| Chloroethane | 0.1771 | 0.1718 | 125.00 | 121.25 | 3.00 | 91.21 | Avg RF |
| Trichlorofluoromethane | 0.4441 | 0.4419 | 125.00 | 124.38 | 0.49 | 88.74 | Avg RF |
| 1,1-Dichloroethene | 0.2518 | 0.2602 | 125.00 | 129.18 | -3.34 | 99.23 | Avg RF |
| Methylene chloride | 0.3712 | 0.3763 | 125.00 | 126.70 | -1.36 | 105.47 | Avg RF |
| trans-1,2-Dichloroethene | 0.2569 | 0.2719 | 125.00 | 132.27 | -5.82 | 102.66 | Avg RF |
| Methyl tert-butyl ether (MTBE) | 0.3321 | 0.3450 | 125.00 | 129.87 | -3.90 | 94.07 | Avg RF |
| 1,1-Dichloroethane | 0.4782 | 0.5253 | 125.00 | 137.31 | -9.85 | 107.06 | Avg RF |
| 2,2-Dichloropropane | 0.3583 | 0.3831 | 125.00 | 133.65 | -6.92 | 104.02 | Avg RF |
| cis-1,2-Dichloroethene | 0.2605 | 0.2863 | 125.00 | 137.39 | -9.91 | 108.49 | Avg RF |
| Methyl ethyl ketone | 0.0353 | 0.0362 # | 1250.00 | 1283.80 | -2.70 | 101.98 | Avg RF |
| Bromochloromethane | 0.1079 | 0.1215 | 125.00 | 140.79 | -12.63 | 109.81 | Avg RF |
| Chloroform | 0.4759 | 0.4899 | 125.00 | 128.66 | -2.93 | 103.39 | Avg RF |
| 1,1,1-Trichloroethane | 0.4460 | 0.4612 | 125.00 | 129.27 | -3.41 | 100.39 | Avg RF |
| Dibromofluoromethane | 0.2355 | 0.2654 | 250.00 | 281.66 | -12.67 | 225.32 | Avg RF |
| Carbon tetrachloride | 0.4394 | 0.4508 | 125.00 | 128.23 | -2.58 | 98.84 | Avg RF |
| 1,1-Dichloropropene | 0.3792 | 0.3963 | 125.00 | 130.64 | -4.51 | 100.42 | Avg RF |
| 1,2-Dichloroethane-d4 | 0.1017 | 0.1183 | 250.00 | 290.73 | -16.29 | 229.53 | Avg RF |
| Benzene | 0.9954 | 1.0777 | 125.00 | 135.33 | -8.26 | 106.55 | Avg RF |
| 1,2-Dichloroethane | 0.2693 | 0.2909 | 125.00 | 135.04 | -8.03 | 105.19 | Avg RF |
| -----ISTD----- | | | | | | | |
| Chlorobenzene-d5 | 0.7540 | 0.7933 | 125.00 | 131.53 | -5.22 | 100.63 | Avg RF |
| Trichloroethene | 0.6632 | 0.7231 | 125.00 | 136.30 | -9.04 | 105.54 | Avg RF |
| 1,2-Dichloropropane | 0.2803 | 0.3053 | 125.00 | 136.15 | -8.92 | 108.77 | Avg RF |
| Dibromomethane | 0.7735 | 0.8310 | 125.00 | 134.30 | -7.44 | 104.00 | Avg RF |
| Bromodichloromethane | 0.8745 | 0.9229 | 125.00 | 131.92 | -5.54 | 103.23 | Avg RF |
| cis-1,3-Dichloropropene | 2.4091 | 2.6773 | 250.00 | 277.83 | -11.13 | 216.40 | Avg RF |
| Toluene-d8 | 1.6274 | 1.7767 | 125.00 | 136.47 | -9.18 | 105.10 | Avg RF |
| Toluene | 0.6225 | 0.7254 | 125.00 | 145.67 | -16.53 | 113.26 | Avg RF |
| trans-1,3-Dichloropropene | 0.3242 | 0.3608 | 125.00 | 139.08 | -11.27 | 111.90 | Avg RF |
| 1,1,2-Trichloroethane | 0.6639 | 0.6868 | 125.00 | 129.31 | -3.45 | 101.88 | Avg RF |
| Tetrachloroethene | | | | | | | |

Continuing Calibration Report

| Target Compound | AvgRF/R2 | CC RF | Exp. Conc | Calc. Conc | %Dev | Area% | Curve Fit |
|---------------------------|----------------|--------|-----------|------------|--------|--------|-----------|
| 1,3-Dichloropropane | 0.6378 | 0.7168 | 125.00 | 140.48 | -12.39 | 107.88 | Avg RF |
| Chlorodibromomethane | 0.5068 | 0.5640 | 125.00 | 139.12 | -11.30 | 108.84 | Avg RF |
| 1,2-Dibromoethane | 0.3545 | 0.3884 | 125.00 | 136.93 | -9.55 | 108.48 | Avg RF |
| Chlorobenzene | 1.7817 | 1.8910 | 125.00 | 132.67 | -6.14 | 103.84 | Avg RF |
| 1,1,1,2-Tetrachloroethane | 0.6228 | 0.6652 | 125.00 | 133.51 | -6.81 | 105.93 | Avg RF |
| Ethylbenzene | 3.0900 | 3.2737 | 125.00 | 132.43 | -5.95 | 102.10 | Avg RF |
| m+p-Xylenes | 1.2008 | 1.2890 | 250.00 | 268.37 | -7.35 | 101.30 | Avg RF |
| o-Xylene | 1.0690 | 1.1451 | 125.00 | 133.90 | -7.12 | 102.64 | Avg RF |
| Styrene | 1.7211 | 1.9345 | 125.00 | 140.50 | -12.40 | 104.35 | Avg RF |
| 1,4-Dichlorobenzene-d4 | -----ISTD----- | | | | | | |
| Bromoform | 0.3199 | 0.3590 | 125.00 | 140.27 | -12.21 | 111.32 | Avg RF |
| p-Bromofluorobenzene | 0.9159 | 0.9772 | 250.00 | 266.74 | -6.70 | 207.73 | Avg RF |
| Bromobenzene | 0.8091 | 0.8723 | 125.00 | 134.77 | -7.82 | 103.60 | Avg RF |
| 1,1,2,2-Tetrachloroethane | 0.4657 | 0.5225 | 125.00 | 140.25 | -12.20 | 111.41 | Avg RF |
| 1,2,3-Trichloropropane | 0.1246 | 0.1415 | 125.00 | 141.96 | -13.57 | 51.90 | Avg RF |
| 2-Chlorotoluene | 0.8050 | 0.8513 | 125.00 | 132.18 | -5.75 | 100.94 | Avg RF |
| 4-Chlorotoluene | 2.6247 | 2.8655 | 125.00 | 136.47 | -9.17 | 103.53 | Avg RF |
| 1,3-Dichlorobenzene | 1.4756 | 1.5333 | 125.00 | 129.89 | -3.91 | 101.54 | Avg RF |
| 1,4-Dichlorobenzene | 1.5046 | 1.5813 | 125.00 | 131.37 | -5.10 | 101.59 | Avg RF |
| 1,2-Dichlorobenzene | 1.2470 | 1.2845 | 125.00 | 128.76 | -3.00 | 102.44 | Avg RF |

A -- against Average; M -- against Mid Point; P -- against Previous CC in the Method;

Continuing Calibration Report

Batch Name D:\Org\Data\VOA5975C\VG010522\QuantResults\VG010522_8260B.batch.bin
Method File \\MASSHUNTER\Org\Data\Methods\Quant\VOA5975C\VOA5975C_010422_CAL\VOA5975C_8260B_SHT_DoD_L4_010422.m
Daily CC D:\Org\Data\VOA5975C\VG01052205JAN27.D

| Level name | Injection Time | Calibration Files |
|------------|---------------------|--|
| 1 | 1/4/2022 3:33:04 PM | D:\Org\Data\VOA5975C\VG010422\04JAN10.D |
| 2 | 1/4/2022 4:00:35 PM | D:\Org\Data\VOA5975C\VG010422\04JAN11.D |
| 3 | 1/4/2022 4:28:05 PM | D:\Org\Data\VOA5975C\VG010422\04JAN12.D |
| 4 | 1/4/2022 4:55:32 PM | D:\Org\Data\VOA5975C\VG010422\04JAN13.D |
| 5 | 1/4/2022 5:50:25 PM | D:\Org\Data\VOA5975C\VG010422\04JAN15.D |
| 6 | 1/4/2022 6:45:10 PM | D:\Org\Data\VOA5975C\VG010422\04JAN17.D |
| 7 | 1/4/2022 7:39:45 PM | D:\Org\Data\VOA5975C\VG010422\04JAN19.D |
| 8 | 1/4/2022 8:34:31 PM | D:\Org\Data\VOA5975C\VG010422\04JAN21.D |
| CC | 1/5/2022 9:55:17 PM | D:\Org\Data\VOA5975C\VG010522\05JAN27.D <===== |

| ISTD Compound: | Avg Resp | Mid Resp | CC Resp | Area% | A/M |
|------------------------|----------|----------|---------|--------|-----|
| Fluorobenzene | 805964 | 778120 | 792987 | 101.91 | M |
| Chlorobenzene-d5 | 305684 | 300356 | 303776 | 101.14 | M |
| 1,4-Dichlorobenzene-d4 | 252451 | 248636 | 251051 | 100.97 | M |

| Target Compound | AvgRF/R2 | CC RF | Exp. Conc | Calc. Conc | %Dev | Area% | Curve Fit |
|--------------------------------|----------|----------|-----------|------------|--------|--------|-----------|
| -----ISTD----- | | | | | | | |
| Dichlorodifluoromethane | 0.3276 | 0.3166 | 125.00 | 120.81 | 3.35 | 91.01 | Avg RF |
| Chloromethane | 0.3976 | 0.3723 | 125.00 | 117.05 | 6.36 | 91.92 | Avg RF |
| Vinyl chloride | 0.3578 | 0.3417 | 125.00 | 119.38 | 4.50 | 91.32 | Avg RF |
| Bromomethane | 0.1600 | 0.1583 | 125.00 | 123.70 | 1.04 | 96.34 | Avg RF |
| Chloroethane | 0.1771 | 0.1566 | 125.00 | 110.53 | 11.57 | 86.95 | Avg RF |
| Trichlorofluoromethane | 0.4441 | 0.4369 | 125.00 | 122.98 | 1.62 | 91.75 | Avg RF |
| 1,1-Dichloroethene | 0.2518 | 0.2421 | 125.00 | 120.16 | 3.87 | 96.52 | Avg RF |
| Methylene chloride | 0.3712 | 0.3348 | 125.00 | 112.75 | 9.80 | 98.14 | Avg RF |
| trans-1,2-Dichloroethene | 0.2569 | 0.2520 | 125.00 | 122.59 | 1.92 | 99.50 | Avg RF |
| Methyl tert-butyl ether (MTBE) | 0.3321 | 0.3128 | 125.00 | 117.73 | 5.82 | 89.17 | Avg RF |
| 1,1-Dichloroethane | 0.4782 | 0.4676 | 125.00 | 122.23 | 2.22 | 99.65 | Avg RF |
| 2,2-Dichloropropane | 0.3583 | 0.3412 | 125.00 | 119.01 | 4.79 | 96.86 | Avg RF |
| cis-1,2-Dichloroethene | 0.2605 | 0.2536 | 125.00 | 121.69 | 2.65 | 100.48 | Avg RF |
| Methyl ethyl ketone | 0.0353 | 0.0319 # | 1250.00 | 1129.33 | 9.65 | 93.81 | Avg RF |
| Bromochloromethane | 0.1079 | 0.1039 | 125.00 | 120.31 | 3.75 | 98.13 | Avg RF |
| Chloroform | 0.4759 | 0.4426 | 125.00 | 116.26 | 6.99 | 97.70 | Avg RF |
| 1,1,1-Trichloroethane | 0.4460 | 0.4326 | 125.00 | 121.23 | 3.02 | 98.45 | Avg RF |
| Dibromofluoromethane | 0.2355 | 0.2553 | 250.00 | 270.98 | -8.39 | 226.68 | Avg RF |
| Carbon tetrachloride | 0.4394 | 0.4283 | 125.00 | 121.83 | 2.54 | 98.20 | Avg RF |
| 1,1-Dichloropropene | 0.3792 | 0.3688 | 125.00 | 121.57 | 2.74 | 97.72 | Avg RF |
| 1,2-Dichloroethane-d4 | 0.1017 | 0.1133 | 250.00 | 278.44 | -11.38 | 229.87 | Avg RF |
| Benzene | 0.9954 | 0.9757 | 125.00 | 122.53 | 1.98 | 100.89 | Avg RF |
| 1,2-Dichloroethane | 0.2693 | 0.2584 | 125.00 | 119.94 | 4.05 | 97.70 | Avg RF |
| -----ISTD----- | | | | | | | |
| Chlorobenzene-d5 | | | | | | | |
| Trichloroethene | 0.7540 | 0.7302 | 125.00 | 121.06 | 3.15 | 97.19 | Avg RF |
| 1,2-Dichloropropane | 0.6632 | 0.6135 | 125.00 | 115.63 | 7.50 | 93.95 | Avg RF |
| Dibromomethane | 0.2803 | 0.2649 | 125.00 | 118.13 | 5.49 | 99.02 | Avg RF |
| Bromodichloromethane | 0.7735 | 0.7365 | 125.00 | 119.03 | 4.78 | 96.72 | Avg RF |
| cis-1,3-Dichloropropene | 0.8745 | 0.7928 | 125.00 | 113.32 | 9.34 | 93.05 | Avg RF |
| Toluene-d8 | 2.4091 | 2.6515 | 250.00 | 275.15 | -10.06 | 224.87 | Avg RF |
| Toluene | 1.6274 | 1.5859 | 125.00 | 121.82 | 2.55 | 98.43 | Avg RF |
| trans-1,3-Dichloropropene | 0.6225 | 0.5956 | 125.00 | 119.59 | 4.33 | 97.56 | Avg RF |
| 1,1,2-Trichloroethane | 0.3242 | 0.2992 | 125.00 | 115.36 | 7.71 | 97.38 | Avg RF |
| Tetrachloroethene | 0.6639 | 0.6327 | 125.00 | 119.13 | 4.69 | 98.48 | Avg RF |


Continuing Calibration Report

| Target Compound | AvgRF/R2 | CC RF | Exp. Conc | Calc. Conc | %Dev | Area% | Curve Fit |
|---------------------------|----------------|--------|-----------|------------|-------|--------|-----------|
| 1,3-Dichloropropane | 0.6378 | 0.6039 | 125.00 | 118.37 | 5.30 | 95.37 | Avg RF |
| Chlorodibromomethane | 0.5068 | 0.4788 | 125.00 | 118.11 | 5.51 | 96.95 | Avg RF |
| 1,2-Dibromoethane | 0.3545 | 0.3255 | 125.00 | 114.75 | 8.20 | 95.39 | Avg RF |
| Chlorobenzene | 1.7817 | 1.7190 | 125.00 | 120.60 | 3.52 | 99.04 | Avg RF |
| 1,1,1,2-Tetrachloroethane | 0.6228 | 0.5904 | 125.00 | 118.50 | 5.20 | 98.65 | Avg RF |
| Ethylbenzene | 3.0900 | 2.9865 | 125.00 | 120.82 | 3.35 | 97.73 | Avg RF |
| m+p-Xylenes | 1.2008 | 1.2057 | 250.00 | 251.02 | -0.41 | 99.41 | Avg RF |
| o-Xylene | 1.0690 | 1.0524 | 125.00 | 123.06 | 1.55 | 98.97 | Avg RF |
| Styrene | 1.7211 | 1.7476 | 125.00 | 126.93 | -1.54 | 98.91 | Avg RF |
| 1,4-Dichlorobenzene-d4 | -----ISTD----- | | | | | | |
| Bromoform | 0.3199 | 0.3108 | 125.00 | 121.44 | 2.85 | 99.61 | Avg RF |
| p-Bromofluorobenzene | 0.9159 | 0.9759 | 250.00 | 266.38 | -6.55 | 214.40 | Avg RF |
| Bromobenzene | 0.8091 | 0.8046 | 125.00 | 124.30 | 0.56 | 98.76 | Avg RF |
| 1,1,2,2-Tetrachloroethane | 0.4657 | 0.4463 | 125.00 | 119.79 | 4.17 | 98.35 | Avg RF |
| 1,2,3-Trichloropropane | 0.1246 | 0.1103 | 125.00 | 110.62 | 11.51 | 41.80 | Avg RF |
| 2-Chlorotoluene | 0.8050 | 0.8090 | 125.00 | 125.62 | -0.49 | 99.15 | Avg RF |
| 4-Chlorotoluene | 2.6247 | 2.6323 | 125.00 | 125.36 | -0.29 | 98.30 | Avg RF |
| 1,3-Dichlorobenzene | 1.4756 | 1.4289 | 125.00 | 121.05 | 3.16 | 97.80 | Avg RF |
| 1,4-Dichlorobenzene | 1.5046 | 1.4106 | 125.00 | 117.20 | 6.24 | 93.67 | Avg RF |
| 1,2-Dichlorobenzene | 1.2470 | 1.1829 | 125.00 | 118.57 | 5.14 | 97.51 | Avg RF |

A -- against Average; M -- against Mid Point; P -- against Previous CC in the Method;

Quantitation Results Report (QT Reviewed)

| | | | |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File | 05JAN03.D | Operator | MSC |
| Acq. Method | 5975CACQF.M | Acq. Date-Time | 1/5/2022 10:28:43 AM |
| Sample Name | CCV010522_ | Instrument | VOA5975C |
| Vial | 3 | Multiplier | 1.00 |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m | Comment | |
| Tune File | BFB_Atune3.u | Tune Date | 10/11/2021 4:02:00 PM |
| Batch Name | VG010522_8260B.batch.bin | Last Calib Update | 2/28/2022 2:48:47 PM |
| Ref Library | \\MASSHUNTER\Org\Library\NIST129K.I | | |



| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|--------------------|-------|----------|
| Internal Standards | | | | | | |
| M Fluorobenzene | 6.621 | 96.0 | 758322 | 250.0000 | ng | -0.003 |
| M Chlorobenzene-d5 | 9.774 | 82.0 | 289518 | 250.0000 | ng | 0.003 |
| M 1,4-Dichlorobenzene-d4 | 12.100 | 152.0 | 242905 | 250.0000 | ng | 0.000 |
| System Monitoring Compounds | | | | | | |
| S Dibromofluoromethane | 5.848 | 113.0 | 201225 | 281.6635 | ng | 0.003 |
| Spiked Amount: 250.000 | Range: 80.0 - 119.0% | | | Recovery = 112.67% | | |
| S 1,2-Dichloroethane-d4 | 6.236 | 67.0 | 89713 | 290.7320 | ng | 0.003 |
| Spiked Amount: 250.000 | Range: 81.0 - 118.0% | | | Recovery = 116.29% | | |
| S Toluene-d8 | 8.319 | 98.0 | 775126 | 277.8286 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 89.0 - 112.0% | | | Recovery = 111.13% | | |
| S p-Bromofluorobenzene | 10.951 | 95.0 | 237370 | 266.7422 | ng | -0.003 |
| Spiked Amount: 250.000 | Range: 85.0 - 114.0% | | | Recovery = 106.70% | | |
| Target Compounds | | | | | | |
| T Dichlorodifluoromethane | 1.244 | 85.0 | 120875 | 121.6377 | ng | 99 |
| T Chloromethane | 1.414 | 50.0 | 146389 | 121.3695 | ng | 98 |
| T Vinyl chloride | 1.498 | 62.0 | 134667 | 124.0834 | ng | 89 |
| T Bromomethane | 1.799 | 96.0 | 63447 | 130.7402 | ng | 97 |
| T Chloroethane | 1.897 | 64.0 | 65145 | 121.2486 | ng | 99 |
| T Trichlorofluoromethane | 2.148 | 101.0 | 167554 | 124.3824 | ng | 99 |
| T 1,1-Dichloroethene | 2.705 | 96.0 | 98670 | 129.1761 | ng | 100 |
| T Methylene chloride | 3.333 | 49.0 | 142665 | 126.6979 | ng | 100 |
| T trans-1,2-Dichloroethene | 3.718 | 96.0 | 103078 | 132.2722 | ng | 99 |
| T Methyl tert-butyl ether (MTBE) | 3.748 | 73.0 | 130816 | 129.8706 | ng | 99 |
| T 1,1-Dichloroethane | 4.381 | 63.0 | 199178 | 137.3114 | ng | 98 |
| T 2,2-Dichloropropane | 5.196 | 77.0 | 145269 | 133.6522 | ng | 98 |
| T cis-1,2-Dichloroethene | 5.212 | 96.0 | 108548 | 137.3875 | ng | 96 |
| T Methyl ethyl ketone | 5.279 | 43.0 | 137392 | 1283.7998 | ng | 99 |
| T Bromochloromethane | 5.519 | 128.0 | 46083 | 140.7927 | ng | 97 |
| T Chloroform | 5.650 | 83.0 | 185738 | 128.6627 | ng | 100 |


Quantitation Results Report (QT Reviewed)

| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|-----------------------------|--------|-------|--------|----------|-------|----------|
| T 1,1,1-Trichloroethane | 5.831 | 97.0 | 174885 | 129.2681 | ng | 99 |
| T Carbon tetrachloride | 6.029 | 117.0 | 170926 | 128.2311 | ng | 98 |
| T 1,1-Dichloropropene | 6.040 | 75.0 | 150274 | 130.6385 | ng | 99 |
| T Benzene | 6.280 | 78.0 | 408605 | 135.3309 | ng | 100 |
| T 1,2-Dichloroethane | 6.319 | 62.0 | 110298 | 135.0368 | ng | 98 |
| T Trichloroethene | 7.025 | 95.0 | 114844 | 131.5285 | ng | 98 |
| T 1,2-Dichloropropane | 7.273 | 63.0 | 104682 | 136.2951 | ng | 99 |
| T Dibromomethane | 7.393 | 93.0 | 44191 | 136.1521 | ng | 97 |
| T Bromodichloromethane | 7.585 | 83.0 | 120295 | 134.2956 | ng | 98 |
| T cis-1,3-Dichloropropene | 8.057 | 75.0 | 133603 | 131.9196 | ng | 98 |
| T Toluene | 8.386 | 92.0 | 257200 | 136.4742 | ng | 98 |
| T trans-1,3-Dichloropropene | 8.637 | 75.0 | 105011 | 145.6663 | ng | 96 |
| T 1,1,2-Trichloroethane | 8.818 | 83.0 | 52225 | 139.0820 | ng | 96 |
| T Tetrachloroethene | 8.935 | 163.8 | 99420 | 129.3096 | ng | 97 |
| T 1,3-Dichloropropane | 8.980 | 76.0 | 103760 | 140.4835 | ng | 99 |
| T Chlorodibromomethane | 9.203 | 129.0 | 81647 | 139.1249 | ng | 99 |
| T 1,2-Dibromoethane | 9.303 | 107.0 | 56221 | 136.9319 | ng | 99 |
| T Chlorobenzene | 9.802 | 112.0 | 273742 | 132.6730 | ng | 99 |
| T 1,1,1,2-Tetrachloroethane | 9.889 | 131.0 | 96292 | 133.5071 | ng | 99 |
| T Ethylbenzene | 9.919 | 91.0 | 473903 | 132.4334 | ng | 99 |
| T m+p-Xylenes | 10.037 | 106.0 | 373201 | 268.3696 | ng | 98 |
| T o-Xylene | 10.433 | 106.0 | 165769 | 133.9037 | ng | 99 |
| T Styrene | 10.449 | 104.0 | 280042 | 140.5011 | ng | 99 |
| T Bromoform | 10.622 | 172.5 | 43600 | 140.2668 | ng | 99 |
| T Bromobenzene | 11.093 | 156.0 | 105945 | 134.7722 | ng | 99 |
| T 1,1,2,2-Tetrachloroethane | 11.110 | 83.0 | 63459 | 140.2540 | ng | 97 |
| T 1,2,3-Trichloropropane | 11.149 | 110.0 | 17186 | 141.9567 | ng | 97 |
| T 2-Chlorotoluene | 11.289 | 126.0 | 103391 | 132.1845 | ng | 98 |
| T 4-Chlorotoluene | 11.400 | 91.0 | 348025 | 136.4682 | ng | 100 |
| T 1,3-Dichlorobenzene | 12.030 | 146.0 | 186227 | 129.8930 | ng | 99 |
| T 1,4-Dichlorobenzene | 12.123 | 146.0 | 192050 | 131.3733 | ng | 98 |
| T 1,2-Dichlorobenzene | 12.493 | 146.0 | 156006 | 128.7555 | ng | 98 |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------------|----------|------|----------|--------|------|--------|-------|-------|
| Dichlorodifluoromethane | 121.6377 | 1.24 | 0.00 | 120875 | 87.0 | 32.9 | 2.3 | 62.3 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------|----------|------|----------|--------|------|--------|-------|-------|
| Chloromethane | 121.3695 | 1.41 | 0.01 | 146389 | 52.0 | 33.2 | 2.1 | 62.1 |







| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------|----------|------|----------|--------|------|--------|-------|-------|
| Vinyl chloride | 124.0834 | 1.50 | 0.00 | 134667 | 64.0 | 36.1 | 0.0 | 59.9 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|----------|------|----------|-------|------|--------|-------|-------|
| Bromomethane | 130.7402 | 1.80 | 0.00 | 63447 | 94.0 | 108.2 | 74.6 | 134.6 |




Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------------|----------|------|----------|--------|------|--------|-------|-------|
| trans-1,2-Dichloroethene | 132.2722 | 3.72 | 0.00 | 103078 | 61.0 | 155.5 | 123.9 | 183.9 |
| | | | | | 98.0 | 66.0 | 35.7 | 95.7 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------------------|----------|------|----------|--------|------|--------|-------|-------|
| Methyl tert-butyl ether (MTBE) | 129.8706 | 3.75 | -0.01 | 130816 | 57.0 | 25.0 | 0.0 | 54.6 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1-Dichloroethane | 137.3114 | 4.38 | 0.00 | 199178 | 65.0 | 31.0 | 2.1 | 62.1 |
| | | | | | 83.0 | 12.6 | 0.0 | 43.7 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 2,2-Dichloropropane | 133.6522 | 5.20 | 0.00 | 145269 | 41.0 | 68.6 | 36.5 | 96.5 |
| | | | | | 97.0 | 23.6 | 0.0 | 53.2 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,2-Dichloroethene | 137.3875 | 5.21 | 0.00 | 108548 | 61.0 | 161.2 | 137.2 | 197.2 |
| | | | | | 98.0 | 64.7 | 37.3 | 97.3 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|-----------|------|----------|--------|------|--------|-------|-------|
| Methyl ethyl ketone | 1283.7998 | 5.28 | 0.00 | 137392 | 72.0 | 21.0 | 0.0 | 51.3 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|-------|------|--------|-------|-------|
| Bromochloromethane | 140.7927 | 5.52 | 0.00 | 46083 | 49.0 | 178.7 | 152.9 | 212.9 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|------|--------|-------|-------|
| Chloroform | 128.6627 | 5.65 | 0.00 | 185738 | 85.0 | 66.0 | 36.0 | 96.0 |




| | | | | | | | | |
|-----------------------|----------|------|------|--------|------|------|------|------|
| 1,1,1-Trichloroethane | 129.2681 | 5.83 | 0.00 | 174885 | 99.0 | 63.8 | 34.7 | 94.7 |
| | | | | | 61.0 | 48.8 | 18.1 | 78.1 |



| | | | | | | | | |
|----------------------|----------|------|------|--------|-------|------|-----|------|
| Dibromofluoromethane | 281.6635 | 5.85 | 0.00 | 201225 | 191.5 | 21.4 | 0.0 | 53.1 |
|----------------------|----------|------|------|--------|-------|------|-----|------|




| | | | | | | | | |
|----------------------|----------|------|------|--------|-------|------|------|-------|
| Carbon tetrachloride | 128.2311 | 6.03 | 0.01 | 170926 | 119.0 | 94.8 | 67.2 | 127.2 |
| | | | | | 121.0 | 30.6 | 0.1 | 60.1 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|-------|--------|-------|-------|
| 1,1-Dichloropropene | 130.6385 | 6.04 | 0.00 | 150274 | 110.0 | 36.1 | 5.9 | 65.9 |
| | | | | | 77.0 | 31.4 | 0.1 | 60.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 290.7320 | 6.24 | 0.00 | 89713 | 65.0 | 196.4 | 166.5 | 226.5 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|------|----------|--------|------|--------|-------|-------|
| Benzene | 135.3309 | 6.28 | 0.00 | 408605 | 77.0 | 23.7 | 0.0 | 53.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloroethane | 135.0368 | 6.32 | 0.00 | 110298 | 64.0 | 31.3 | 0.0 | 59.9 |
| | | | | | 98.0 | 7.8 | 0.0 | 37.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|----------|------|----------|--------|-------|--------|-------|-------|
| Trichloroethene | 131.5285 | 7.02 | -0.01 | 114844 | 130.0 | 103.1 | 71.5 | 131.5 |
| | | | | | 97.0 | 65.8 | 34.1 | 94.1 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloropropane | 136.2951 | 7.27 | 0.00 | 104682 | 76.0 | 38.7 | 8.2 | 68.2 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------|----------|------|----------|-------|-------|--------|-------|-------|
| Dibromomethane | 136.1521 | 7.39 | -0.01 | 44191 | 173.5 | 112.5 | 83.7 | 143.7 |
| | | | | | 95.0 | 86.2 | 52.2 | 112.2 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Bromodichloromethane | 134.2956 | 7.59 | 0.00 | 120295 | 85.0 | 66.3 | 34.5 | 94.5 |
| | | | | | 127.0 | 9.8 | 0.0 | 39.6 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,3-Dichloropropene | 131.9196 | 8.06 | 0.00 | 133603 | 39.0 | 54.3 | 23.3 | 83.3 |
| | | | | | 77.0 | 32.6 | 1.0 | 61.0 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 277.8286 | 8.32 | 0.00 | 775126 | 100.0 | 64.3 | 34.4 | 94.4 |
| | | | | | 99.0 | 9.5 | 0.0 | 39.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|------|----------|--------|------|--------|-------|-------|
| Toluene | 136.4742 | 8.39 | 0.00 | 257200 | 91.0 | 172.8 | 145.8 | 205.8 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|----------|------|----------|--------|--------------|--------------|-------------|--------------|
| trans-1,3-Dichloropropene | 145.6663 | 8.64 | 0.00 | 105011 | 39.0 77.0 | 49.2 32.3 | 23.4 2.4 | 83.4 62.4 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|--------------|---------------|--------------|---------------|
| 1,1,2-Trichloroethane | 139.0820 | 8.82 | 0.00 | 52225 | 97.0 85.0 | 111.4 62.8 | 84.6 37.6 | 144.6 97.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------|----------|------|----------|-------|-------|--------|-------|-------|
| Tetrachloroethene | 129.3096 | 8.94 | 0.00 | 99420 | 165.8 | 125.7 | 98.6 | 158.6 |
| | | | | | 129.0 | 88.8 | 61.5 | 121.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,3-Dichloropropane | 140.4835 | 8.98 | 0.00 | 103760 | 78.0 | 32.1 | 2.9 | 62.9 |















| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|-------|-------|--------|-------|-------|
| Chlorodibromomethane | 139.1249 | 9.20 | 0.00 | 81647 | 127.0 | 77.2 | 48.0 | 108.0 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------|----------|------|----------|-------|-------|--------|-------|-------|
| 1,2-Dibromoethane | 136.9319 | 9.30 | 0.00 | 56221 | 109.0 | 93.5 | 64.5 | 124.5 |




Quantitation Results Report (QT Reviewed)

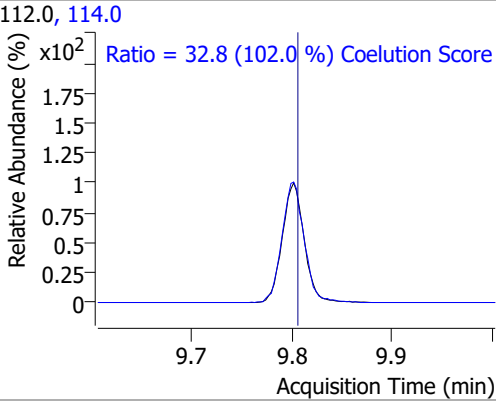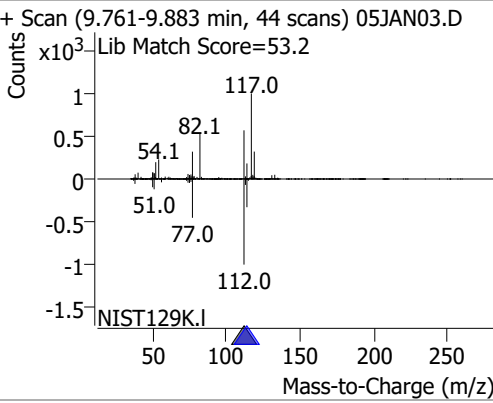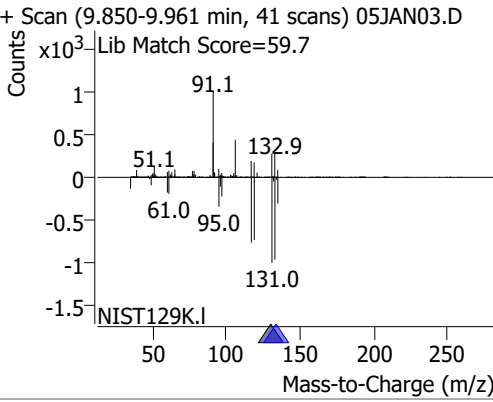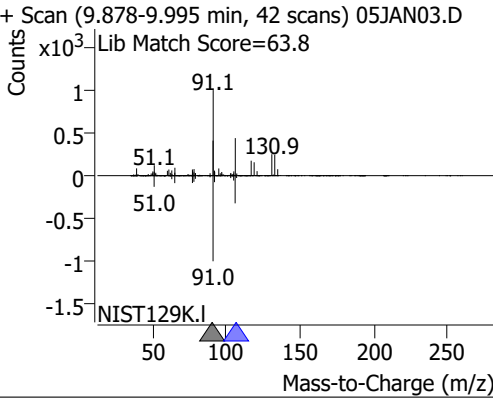
| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--|--|-------|---|--------|-------|---|-------|-------|
| Chlorobenzene | 132.6730 | 9.80 | 0.00 | 273742 | 114.0 | 32.8 | 2.1 | 62.1 |
| + EIC (112.0) Scan 05JAN03.D | | | 112.0, 114.0 | | | + Scan (9.761-9.883 min, 44 scans) 05JAN03.D | | |
|  |  | |  | | | | | |
| Ratio = 32.8 (102.0 %) Coelution Score = | | | | | | | | |
| 1,1,1,2-Tetrachloroethane | 133.5071 | 9.89 | 0.00 | 96292 | 133.0 | 98.0 | 68.6 | 128.6 |
| + EIC (131.0) Scan 05JAN03.D | | | 131.0, 133.0 | | | + Scan (9.850-9.961 min, 41 scans) 05JAN03.D | | |
|  |  | |  | | | | | |
| Ratio = 98.0 (99.3 %) Coelution Score = | | | | | | | | |
| Ethylbenzene | 132.4334 | 9.92 | 0.00 | 473903 | 106.0 | 31.7 | 1.1 | 61.1 |
| + EIC (91.0) Scan 05JAN03.D | | | 91.0, 106.0 | | | + Scan (9.878-9.995 min, 42 scans) 05JAN03.D | | |
|  |  | |  | | | | | |
| Ratio = 31.7 (101.7 %) Coelution Score = | | | | | | | | |
| m+p-Xylenes | 268.3696 | 10.04 | 0.00 | 373201 | 91.0 | 204.5 | 171.4 | 231.4 |
| + EIC (106.0) Scan 05JAN03.D | | | 106.0, 91.0 | | | + Scan (9.998-10.112 min, 42 scans) 05JAN03.D | | |
|  |  | |  | | | | | |
| Ratio = 204.5 (101.5 %) Coelution Score = | | | | | | | | |

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|-------|----------|--------|------|--------|-------|-------|
| o-Xylene | 133.9037 | 10.43 | 0.00 | 165769 | 91.0 | 213.9 | 183.1 | 243.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|-------|----------|--------|------|--------|-------|-------|
| Styrene | 140.5011 | 10.45 | 0.00 | 280042 | 78.0 | 50.0 | 19.6 | 79.6 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------|----------|-------|----------|-------|----------------|--------------|--------------|--------------|
| Bromoform | 140.2668 | 10.62 | -0.01 | 43600 | 170.5 174.5 | 51.4 49.2 | 22.1 20.1 | 82.1 80.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|----------------|--------------|--------------|----------------|
| p-Bromofluorobenzene | 266.7422 | 10.95 | 0.00 | 237370 | 174.0 176.0 | 94.0 93.3 | 61.7 60.6 | 121.7 120.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|----------|-------|----------|--------|-------|--------|-------|-------|
| Bromobenzene | 134.7722 | 11.09 | 0.00 | 105945 | 77.0 | 146.3 | 115.7 | 175.7 |
| | | | | | 158.0 | 97.9 | 66.5 | 126.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|----------|-------|----------|-------|------|--------|-------|-------|
| 1,1,2,2-Tetrachloroethane | 140.2540 | 11.11 | -0.01 | 63459 | 85.0 | 63.5 | 36.2 | 96.2 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|----------|-------|----------|-------|-------|--------|-------|-------|
| 1,2,3-Trichloropropane | 141.9567 | 11.15 | 0.00 | 17186 | 112.0 | 60.9 | 33.5 | 93.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|----------|-------|----------|--------|------|--------|-------|-------|
| 2-Chlorotoluene | 132.1845 | 11.29 | 0.00 | 103391 | 91.0 | 285.7 | 252.3 | 312.3 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 4-Chlorotoluene | 136.4682 | 11.40 | 0.00 | 348025 | 126.0 | 31.9 | 1.7 | 61.7 |



| | | | | | | | | |
|---------------------|----------|-------|------|--------|-------|------|------|------|
| 1,3-Dichlorobenzene | 129.8930 | 12.03 | 0.00 | 186227 | 148.0 | 64.9 | 33.6 | 93.6 |
| | | | | | 111.0 | 39.1 | 9.8 | 69.8 |






| | | | | | | | | |
|---------------------|----------|-------|------|--------|-------|------|------|------|
| 1,4-Dichlorobenzene | 131.3733 | 12.12 | 0.00 | 192050 | 148.0 | 66.0 | 33.1 | 93.1 |
| | | | | | 111.0 | 38.8 | 9.1 | 69.1 |




Quantitation Results Report (QT Reviewed)

| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,2-Dichlorobenzene | 128.7555 | 12.49 | 0.00 | 156006 | 148.0 | 65.4 | 33.9 | 93.9 |
| | | | | | 111.0 | 40.3 | 11.0 | 71.0 |



Quantitation Results Report (QT Reviewed)

| | | | |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File | 05JAN04.D | Operator | MSC |
| Acq. Method | 5975CACQF.M | Acq. Date-Time | 1/5/2022 11:27:34 AM |
| Sample Name | LCS010522_ | Instrument | VOA5975C |
| Vial | 4 | Multiplier | 1.00 |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m | Comment | |
| Tune File | BFB_Atune3.u | Tune Date | 10/11/2021 4:02:00 PM |
| Batch Name | VG010522_8260B.batch.bin | Last Calib Update | 2/28/2022 2:48:47 PM |
| Ref Library | \\MASSHUNTER\Org\Library\NIST129K.I | | |















| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|--------------------|-------|----------|
| Internal Standards | | | | | | |
| M Fluorobenzene | 6.620 | 96.0 | 795901 | 250.0000 | ng | -0.003 |
| M Chlorobenzene-d5 | 9.774 | 82.0 | 307268 | 250.0000 | ng | 0.003 |
| M 1,4-Dichlorobenzene-d4 | 12.100 | 152.0 | 255531 | 250.0000 | ng | 0.000 |
| System Monitoring Compounds | | | | | | |
| S Dibromofluoromethane | 5.845 | 113.0 | 205546 | 274.1273 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 80.0 - 119.0% | | | Recovery = 109.65% | | |
| S 1,2-Dichloroethane-d4 | 6.233 | 67.0 | 91407 | 282.2354 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 81.0 - 118.0% | | | Recovery = 112.89% | | |
| S Toluene-d8 | 8.319 | 98.0 | 806393 | 272.3389 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 89.0 - 112.0% | | | Recovery = 108.94% | | |
| S p-Bromofluorobenzene | 10.951 | 95.0 | 252422 | 269.6410 | ng | -0.003 |
| Spiked Amount: 250.000 | Range: 85.0 - 114.0% | | | Recovery = 107.86% | | |
| Target Compounds | | | | | | |
| T Dichlorodifluoromethane | 1.244 | 85.0 | 113781 | 109.0928 | ng | 100 |
| T Chloromethane | 1.411 | 50.0 | 142248 | 112.3678 | ng | 99 |
| T Vinyl chloride | 1.498 | 62.0 | 137634 | 120.8294 | ng | 89 |
| T Bromomethane | 1.802 | 96.0 | 55806 | 109.5654 | ng | 94 |
| T Chloroethane | 1.897 | 64.0 | 65207 | 115.6337 | ng | 99 |
| T Trichlorofluoromethane | 2.148 | 101.0 | 175235 | 123.9423 | ng | 99 |
| T 1,1-Dichloroethene | 2.700 | 96.0 | 109762 | 136.9127 | ng | 98 |
| T Methylene chloride | 3.333 | 49.0 | 151653 | 128.3209 | ng | 99 |
| T trans-1,2-Dichloroethene | 3.720 | 96.0 | 110475 | 135.0707 | ng | 99 |
| T Methyl tert-butyl ether (MTBE) | 3.754 | 73.0 | 151310 | 143.1239 | ng | 99 |
| T 1,1-Dichloroethane | 4.381 | 63.0 | 211828 | 139.1372 | ng | 99 |
| T 2,2-Dichloropropane | 5.193 | 77.0 | 151230 | 132.5671 | ng | 99 |
| T cis-1,2-Dichloroethene | 5.218 | 96.0 | 111191 | 134.0879 | ng | 99 |
| T Methyl ethyl ketone | 5.279 | 43.0 | 146436 | 1303.7020 | ng | 97 |
| T Bromochloromethane | 5.519 | 128.0 | 46484 | 135.3123 | ng | 99 |
| T Chloroform | 5.653 | 83.0 | 186606 | 123.1607 | ng | 100 |

Quantitation Results Report (QT Reviewed)

| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|-----------------------------|--------|-------|--------|----------|-------|----------|
| T 1,1,1-Trichloroethane | 5.834 | 97.0 | 179093 | 126.1281 | ng | 99 |
| T Carbon tetrachloride | 6.027 | 117.0 | 168794 | 120.6526 | ng | 98 |
| T 1,1-Dichloropropene | 6.038 | 75.0 | 148070 | 122.6447 | ng | 100 |
| T Benzene | 6.277 | 78.0 | 425505 | 134.2741 | ng | 100 |
| T 1,2-Dichloroethane | 6.319 | 62.0 | 109086 | 127.2472 | ng | 96 |
| T Trichloroethene | 7.025 | 95.0 | 118702 | 128.0937 | ng | 98 |
| T 1,2-Dichloropropane | 7.270 | 63.0 | 104508 | 128.2082 | ng | 100 |
| T Dibromomethane | 7.396 | 93.0 | 44870 | 130.2581 | ng | 96 |
| T Bromodichloromethane | 7.585 | 83.0 | 127493 | 134.1093 | ng | 98 |
| T cis-1,3-Dichloropropene | 8.057 | 75.0 | 135033 | 125.6294 | ng | 99 |
| T Toluene | 8.386 | 92.0 | 268829 | 134.4045 | ng | 98 |
| T trans-1,3-Dichloropropene | 8.637 | 75.0 | 105613 | 138.0384 | ng | 97 |
| T 1,1,2-Trichloroethane | 8.818 | 83.0 | 52727 | 132.3073 | ng | 95 |
| T Tetrachloroethene | 8.938 | 163.8 | 104015 | 127.4710 | ng | 98 |
| T 1,3-Dichloropropane | 8.982 | 76.0 | 101295 | 129.2235 | ng | 99 |
| T Chlorodibromomethane | 9.203 | 129.0 | 82588 | 132.5988 | ng | 97 |
| T 1,2-Dibromoethane | 9.303 | 107.0 | 58316 | 133.8295 | ng | 98 |
| T Chlorobenzene | 9.802 | 112.0 | 290162 | 132.5073 | ng | 99 |
| T 1,1,1,2-Tetrachloroethane | 9.892 | 131.0 | 97391 | 127.2305 | ng | 96 |
| T Ethylbenzene | 9.922 | 91.0 | 490561 | 129.1693 | ng | 99 |
| T m+p-Xylenes | 10.037 | 106.0 | 383847 | 260.0800 | ng | 99 |
| T o-Xylene | 10.430 | 106.0 | 172476 | 131.2732 | ng | 99 |
| T Styrene | 10.449 | 104.0 | 285925 | 135.1658 | ng | 98 |
| T Bromoform | 10.628 | 172.5 | 46366 | 141.7950 | ng | 94 |
| T Bromobenzene | 11.096 | 156.0 | 112763 | 136.3576 | ng | 98 |
| T 1,1,2,2-Tetrachloroethane | 11.113 | 83.0 | 63459 | 133.3239 | ng | 97 |
| T 1,2,3-Trichloropropane | 11.149 | 110.0 | 16771 | 131.6839 | ng | 98 |
| T 2-Chlorotoluene | 11.291 | 126.0 | 110603 | 134.4181 | ng | 99 |
| T 4-Chlorotoluene | 11.400 | 91.0 | 365720 | 136.3209 | ng | 99 |
| T 1,3-Dichlorobenzene | 12.033 | 146.0 | 203215 | 134.7385 | ng | 98 |
| T 1,4-Dichlorobenzene | 12.125 | 146.0 | 200166 | 130.1595 | ng | 98 |
| T 1,2-Dichlorobenzene | 12.493 | 146.0 | 168243 | 131.9940 | ng | 99 |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)

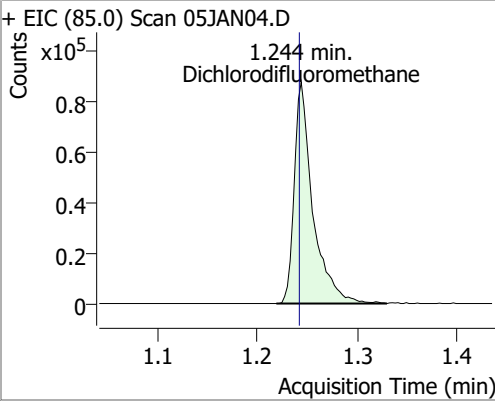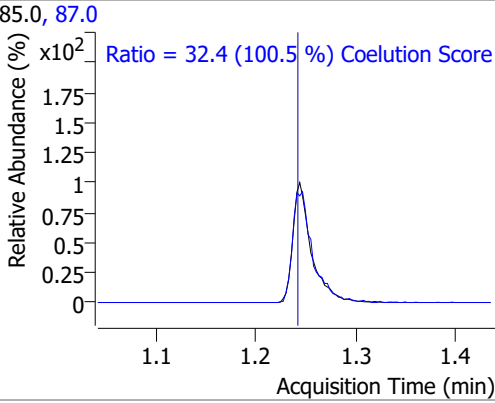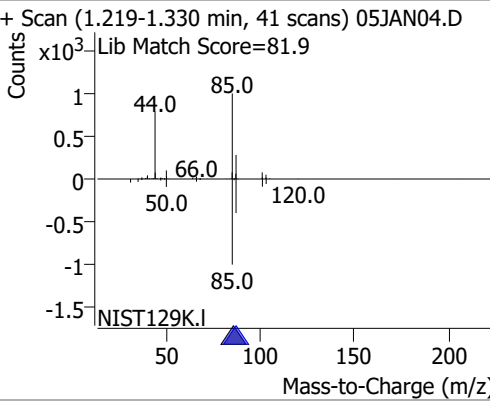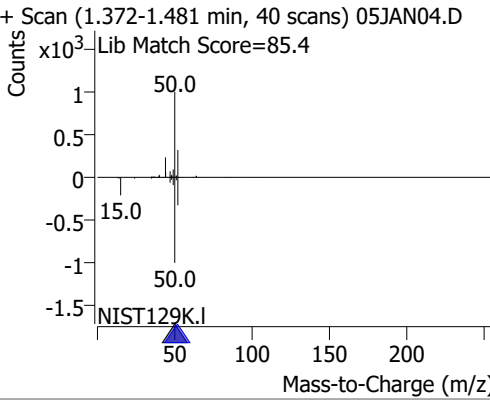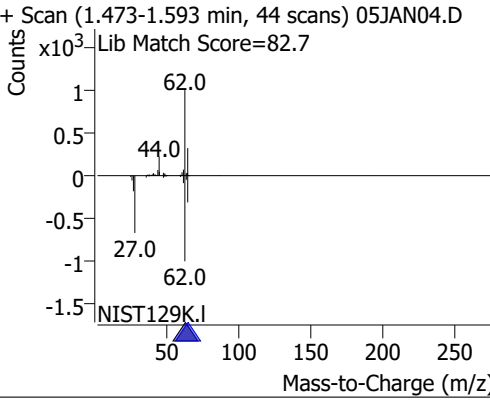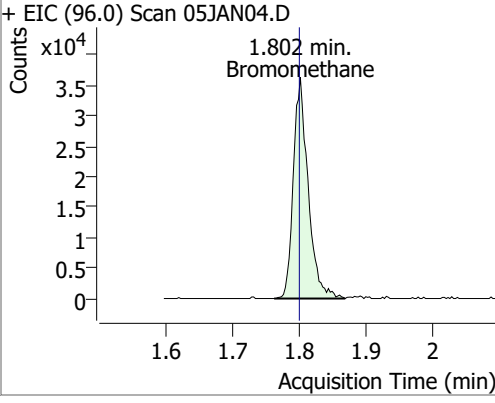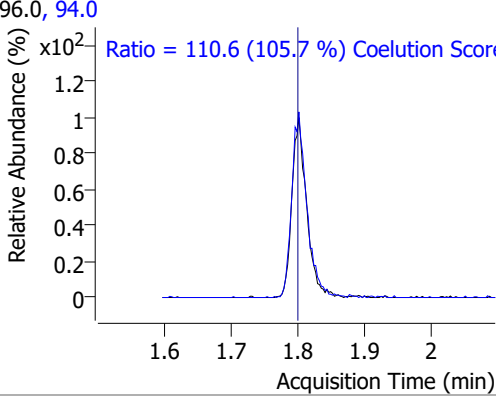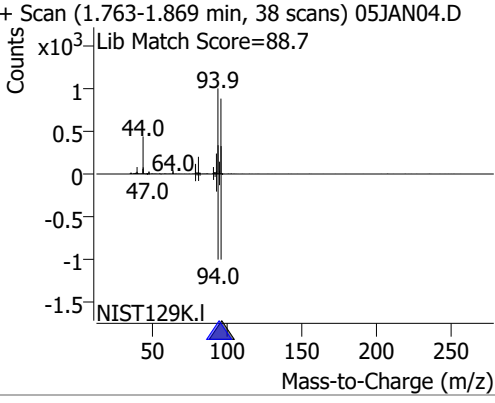
| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---|----------|------|--|--------|------|---|-------|-------|
| Dichlorodifluoromethane | 109.0928 | 1.24 | 0.00 | 113781 | 87.0 | 32.4 | 2.3 | 62.3 |
| + EIC (85.0) Scan 05JAN04.D  | | | 85.0, 87.0  | | | + Scan (1.219-1.330 min, 41 scans) 05JAN04.D Lib Match Score=81.9  | | |
| Chloromethane | 112.3678 | 1.41 | 0.00 | 142248 | 52.0 | 32.6 | 2.1 | 62.1 |
| + EIC (50.0) Scan 05JAN04.D  | | | 50.0, 52.0  | | | + Scan (1.372-1.481 min, 40 scans) 05JAN04.D Lib Match Score=85.4  | | |
| Vinyl chloride | 120.8294 | 1.50 | 0.00 | 137634 | 64.0 | 35.7 | 0.0 | 59.9 |
| + EIC (62.0) Scan 05JAN04.D  | | | 62.0, 64.0  | | | + Scan (1.473-1.593 min, 44 scans) 05JAN04.D Lib Match Score=82.7  | | |
| Bromomethane | 109.5654 | 1.80 | 0.00 | 55806 | 94.0 | 110.6 | 74.6 | 134.6 |
| + EIC (96.0) Scan 05JAN04.D  | | | 96.0, 94.0  | | | + Scan (1.763-1.869 min, 38 scans) 05JAN04.D Lib Match Score=88.7  | | |

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|----------|------|----------|-------|------|--------|-------|-------|
| Chloroethane | 115.6337 | 1.90 | 0.00 | 65207 | 66.0 | 30.7 | 0.1 | 60.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Trichlorofluoromethane | 123.9423 | 2.15 | 0.01 | 175235 | 103.0 | 64.8 | 34.2 | 94.2 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1-Dichloroethene | 136.9127 | 2.70 | 0.00 | 109762 | 61.0 | 177.0 | 150.3 | 210.3 |
| | | | | | 63.0 | 54.8 | 26.7 | 86.7 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| Methylene chloride | 128.3209 | 3.33 | 0.00 | 151653 | 84.0 | 66.1 | 36.9 | 96.9 |
| | | | | | 86.0 | 43.5 | 14.3 | 74.3 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------------|----------|------|----------|--------|------|--------|-------|-------|
| trans-1,2-Dichloroethene | 135.0707 | 3.72 | 0.00 | 110475 | 61.0 | 155.3 | 123.9 | 183.9 |
| | | | | | 98.0 | 64.8 | 35.7 | 95.7 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------------------|----------|------|----------|--------|------|--------|-------|-------|
| Methyl tert-butyl ether (MTBE) | 143.1239 | 3.75 | 0.00 | 151310 | 57.0 | 24.0 | 0.0 | 54.6 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1-Dichloroethane | 139.1372 | 4.38 | 0.00 | 211828 | 65.0 | 31.3 | 2.1 | 62.1 |
| | | | | | 83.0 | 13.2 | 0.0 | 43.7 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 2,2-Dichloropropane | 132.5671 | 5.19 | 0.00 | 151230 | 41.0 | 66.5 | 36.5 | 96.5 |
| | | | | | 97.0 | 24.3 | 0.0 | 53.2 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,2-Dichloroethene | 134.0879 | 5.22 | 0.00 | 111191 | 61.0 | 166.6 | 137.2 | 197.2 |
| | | | | | 98.0 | 68.6 | 37.3 | 97.3 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|-----------|------|----------|--------|------|--------|-------|-------|
| Methyl ethyl ketone | 1303.7020 | 5.28 | 0.00 | 146436 | 72.0 | 22.5 | 0.0 | 51.3 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|-------|------|--------|-------|-------|
| Bromochloromethane | 135.3123 | 5.52 | 0.00 | 46484 | 49.0 | 183.7 | 152.9 | 212.9 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|------|--------|-------|-------|
| Chloroform | 123.1607 | 5.65 | 0.00 | 186606 | 85.0 | 66.2 | 36.0 | 96.0 |




| | | | | | | | | |
|-----------------------|----------|------|------|--------|------|------|------|------|
| 1,1,1-Trichloroethane | 126.1281 | 5.83 | 0.00 | 179093 | 99.0 | 64.4 | 34.7 | 94.7 |
| | | | | | 61.0 | 48.6 | 18.1 | 78.1 |



| | | | | | | | | |
|----------------------|----------|------|------|--------|-------|------|-----|------|
| Dibromofluoromethane | 274.1273 | 5.85 | 0.00 | 205546 | 191.5 | 21.6 | 0.0 | 53.1 |
|----------------------|----------|------|------|--------|-------|------|-----|------|




| | | | | | | | | |
|----------------------|----------|------|------|--------|-------|------|------|-------|
| Carbon tetrachloride | 120.6526 | 6.03 | 0.00 | 168794 | 119.0 | 99.1 | 67.2 | 127.2 |
| | | | | | 121.0 | 31.1 | 0.1 | 60.1 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|-------|--------|-------|-------|
| 1,1-Dichloropropene | 122.6447 | 6.04 | 0.00 | 148070 | 110.0 | 36.1 | 5.9 | 65.9 |
| | | | | | 77.0 | 30.1 | 0.1 | 60.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 282.2354 | 6.23 | 0.00 | 91407 | 65.0 | 200.7 | 166.5 | 226.5 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|------|----------|--------|------|--------|-------|-------|
| Benzene | 134.2741 | 6.28 | 0.00 | 425505 | 77.0 | 23.4 | 0.0 | 53.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloroethane | 127.2472 | 6.32 | 0.00 | 109086 | 64.0 | 32.5 | 0.0 | 59.9 |
| | | | | | 98.0 | 7.8 | 0.0 | 37.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|----------|------|----------|--------|-------|--------|-------|-------|
| Trichloroethene | 128.0937 | 7.02 | -0.01 | 118702 | 130.0 | 103.0 | 71.5 | 131.5 |
| | | | | | 97.0 | 65.8 | 34.1 | 94.1 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloropropane | 128.2082 | 7.27 | 0.00 | 104508 | 76.0 | 38.3 | 8.2 | 68.2 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------|----------|------|----------|-------|-------|--------|-------|-------|
| Dibromomethane | 130.2581 | 7.40 | 0.00 | 44870 | 173.5 | 108.6 | 83.7 | 143.7 |
| | | | | | 95.0 | 84.0 | 52.2 | 112.2 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Bromodichloromethane | 134.1093 | 7.59 | 0.00 | 127493 | 85.0 | 62.6 | 34.5 | 94.5 |
| | | | | | 127.0 | 9.4 | 0.0 | 39.6 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,3-Dichloropropene | 125.6294 | 8.06 | 0.00 | 135033 | 39.0 | 53.5 | 23.3 | 83.3 |
| | | | | | 77.0 | 31.8 | 1.0 | 61.0 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 272.3389 | 8.32 | 0.00 | 806393 | 100.0 | 64.7 | 34.4 | 94.4 |
| | | | | | 99.0 | 9.5 | 0.0 | 39.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|------|----------|--------|------|--------|-------|-------|
| Toluene | 134.4045 | 8.39 | 0.00 | 268829 | 91.0 | 172.3 | 145.8 | 205.8 |



| | | | | | | | | |
|---------------------------|----------|------|------|--------|------|------|------|------|
| trans-1,3-Dichloropropene | 138.0384 | 8.64 | 0.00 | 105613 | 39.0 | 50.4 | 23.4 | 83.4 |
| | | | | | 77.0 | 31.3 | 2.4 | 62.4 |




| | | | | | | | | |
|-----------------------|----------|------|------|-------|------|-------|------|-------|
| 1,1,2-Trichloroethane | 132.3073 | 8.82 | 0.00 | 52727 | 97.0 | 108.5 | 84.6 | 144.6 |
| | | | | | 85.0 | 64.8 | 37.6 | 97.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Tetrachloroethene | 127.4710 | 8.94 | 0.00 | 104015 | 165.8 | 127.4 | 98.6 | 158.6 |
| | | | | | 129.0 | 88.2 | 61.5 | 121.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,3-Dichloropropane | 129.2235 | 8.98 | 0.00 | 101295 | 78.0 | 32.1 | 2.9 | 62.9 |















| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|-------|-------|--------|-------|-------|
| Chlorodibromomethane | 132.5988 | 9.20 | 0.00 | 82588 | 127.0 | 75.4 | 48.0 | 108.0 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------|----------|------|----------|-------|-------|--------|-------|-------|
| 1,2-Dibromoethane | 133.8295 | 9.30 | 0.00 | 58316 | 109.0 | 93.0 | 64.5 | 124.5 |




Quantitation Results Report (QT Reviewed)

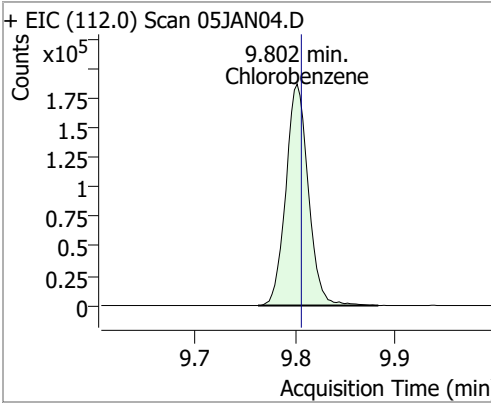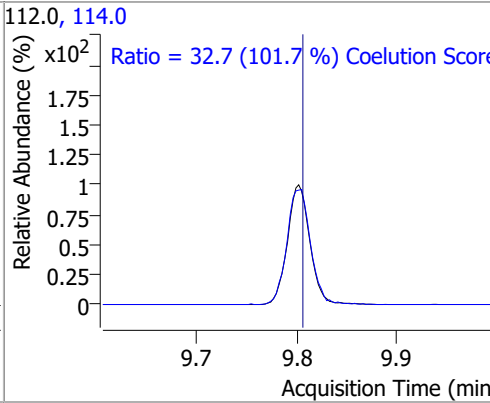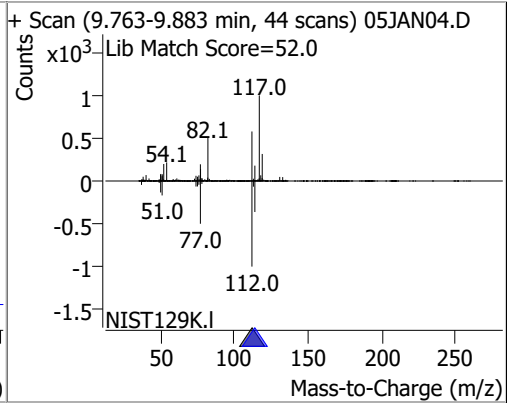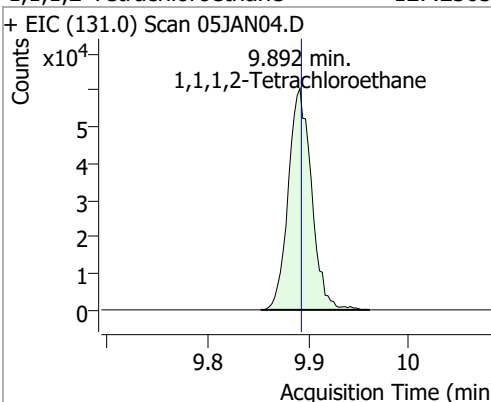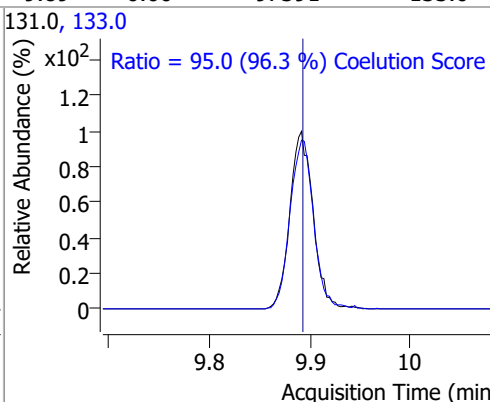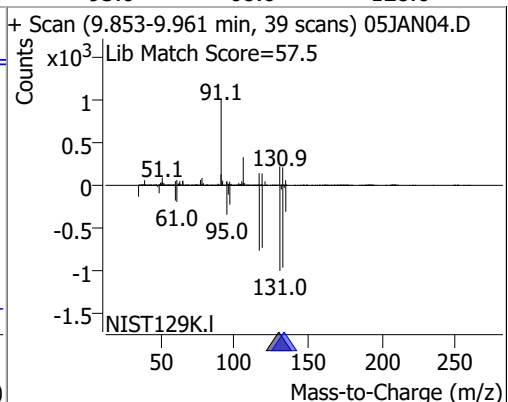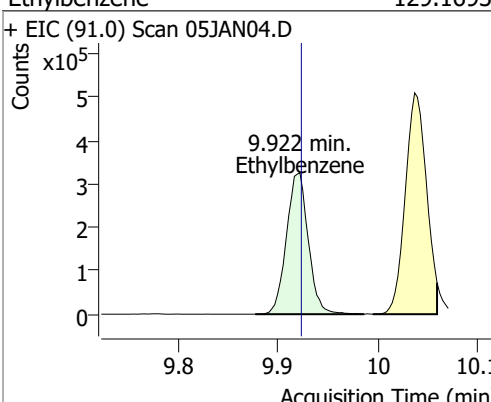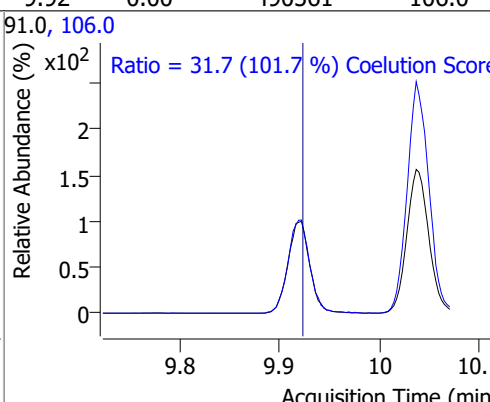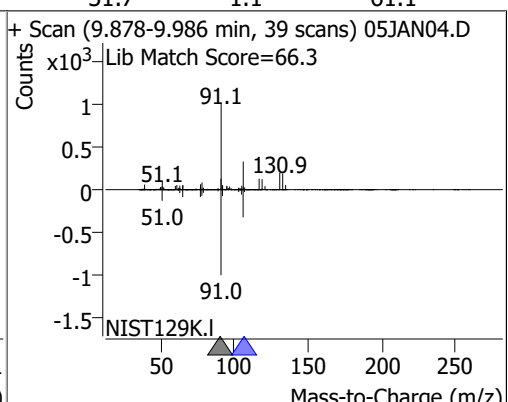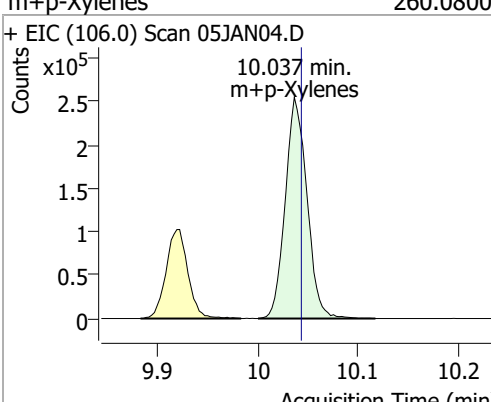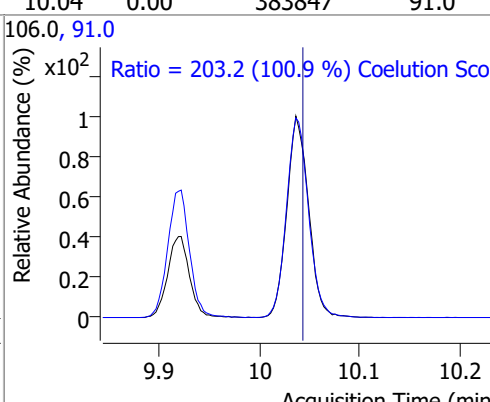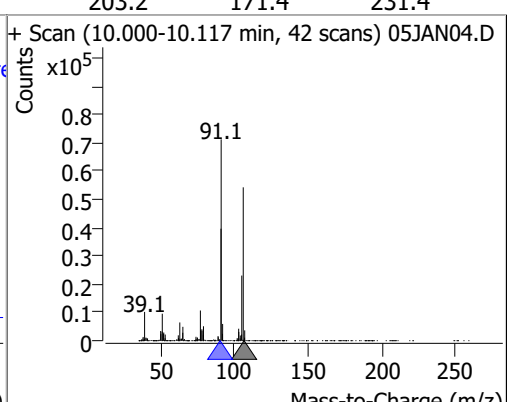
| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--|--|---|--------------|--------|-------|---|-------|-------|
| Chlorobenzene | 132.5073 | 9.80 | 0.00 | 290162 | 114.0 | 32.7 | 2.1 | 62.1 |
| + EIC (112.0) Scan 05JAN04.D | | | 112.0, 114.0 | | | + Scan (9.763-9.883 min, 44 scans) 05JAN04.D | | |
|  |  | Ratio = 32.7 (101.7 %) Coelution Score = | | | |  | | |
| 1,1,1,2-Tetrachloroethane | 127.2305 | 9.89 | 0.00 | 97391 | 133.0 | 95.0 | 68.6 | 128.6 |
| + EIC (131.0) Scan 05JAN04.D | | | 131.0, 133.0 | | | + Scan (9.853-9.961 min, 39 scans) 05JAN04.D | | |
|  |  | Ratio = 95.0 (96.3 %) Coelution Score = | | | |  | | |
| Ethylbenzene | 129.1693 | 9.92 | 0.00 | 490561 | 106.0 | 31.7 | 1.1 | 61.1 |
| + EIC (91.0) Scan 05JAN04.D | | | 91.0, 106.0 | | | + Scan (9.878-9.986 min, 39 scans) 05JAN04.D | | |
|  |  | Ratio = 31.7 (101.7 %) Coelution Score = | | | |  | | |
| m+p-Xylenes | 260.0800 | 10.04 | 0.00 | 383847 | 91.0 | 203.2 | 171.4 | 231.4 |
| + EIC (106.0) Scan 05JAN04.D | | | 106.0, 91.0 | | | + Scan (10.000-10.117 min, 42 scans) 05JAN04.D | | |
|  |  | Ratio = 203.2 (100.9 %) Coelution Score = | | | |  | | |

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|-------|----------|--------|------|--------|-------|-------|
| o-Xylene | 131.2732 | 10.43 | 0.00 | 172476 | 91.0 | 214.1 | 183.1 | 243.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|-------|----------|--------|------|--------|-------|-------|
| Styrene | 135.1658 | 10.45 | 0.00 | 285925 | 78.0 | 51.1 | 19.6 | 79.6 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------|----------|-------|----------|-------|-------|--------|-------|-------|
| Bromoform | 141.7950 | 10.63 | 0.00 | 46366 | 170.5 | 47.3 | 22.1 | 82.1 |
| | | | | | 174.5 | 46.6 | 20.1 | 80.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 269.6410 | 10.95 | 0.00 | 252422 | 174.0 | 92.7 | 61.7 | 121.7 |
| | | | | | 176.0 | 89.5 | 60.6 | 120.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|----------|-------|----------|--------|-------|--------|-------|-------|
| Bromobenzene | 136.3576 | 11.10 | 0.00 | 112763 | 77.0 | 140.8 | 115.7 | 175.7 |
| | | | | | 158.0 | 96.4 | 66.5 | 126.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|----------|-------|----------|-------|------|--------|-------|-------|
| 1,1,2,2-Tetrachloroethane | 133.3239 | 11.11 | 0.00 | 63459 | 85.0 | 63.6 | 36.2 | 96.2 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|----------|-------|----------|-------|-------|--------|-------|-------|
| 1,2,3-Trichloropropane | 131.6839 | 11.15 | 0.00 | 16771 | 112.0 | 62.0 | 33.5 | 93.5 |






| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|----------|-------|----------|--------|------|--------|-------|-------|
| 2-Chlorotoluene | 134.4181 | 11.29 | 0.00 | 110603 | 91.0 | 281.0 | 252.3 | 312.3 |






Quantitation Results Report (QT Reviewed)




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 4-Chlorotoluene | 136.3209 | 11.40 | 0.00 | 365720 | 126.0 | 31.2 | 1.7 | 61.7 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,3-Dichlorobenzene | 134.7385 | 12.03 | 0.00 | 203215 | 148.0 | 62.8 | 33.6 | 93.6 |
| | | | | | 111.0 | 38.4 | 9.8 | 69.8 |






| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,4-Dichlorobenzene | 130.1595 | 12.13 | 0.00 | 200166 | 148.0 | 65.6 | 33.1 | 93.1 |
| | | | | | 111.0 | 39.6 | 9.1 | 69.1 |




Quantitation Results Report (QT Reviewed)

| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,2-Dichlorobenzene | 131.9940 | 12.49 | 0.00 | 168243 | 148.0 | 64.4 | 33.9 | 93.9 |
| | | | | | 111.0 | 40.1 | 11.0 | 71.0 |



Quantitation Results Report (QT Reviewed)

| | | | |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File | 05JAN06.D | Operator | MSC |
| Acq. Method | 5975CACQF.M | Acq. Date-Time | 1/5/2022 12:21:59 PM |
| Sample Name | MBLK010522_ | Instrument | VOA5975C |
| Vial | 6 | Multiplier | 1.00 |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m | Comment | |
| Tune File | BFB_Atune3.u | Tune Date | 10/11/2021 4:02:00 PM |
| Batch Name | VG010522_8260B.batch.bin | Last Calib Update | 2/28/2022 2:48:47 PM |
| Ref Library | \\MASSHUNTER\Org\Library\NIST129K.I | | |



| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|----------|----|------|-------|-------|-------|----------|
|----------|----|------|-------|-------|-------|----------|

Internal Standards

| | | | | | | |
|--------------------------|--------|-------|--------|----------|----|--------|
| M Fluorobenzene | 6.620 | 96.0 | 749177 | 250.0000 | ng | -0.003 |
| M Chlorobenzene-d5 | 9.772 | 82.0 | 294744 | 250.0000 | ng | 0.000 |
| M 1,4-Dichlorobenzene-d4 | 12.103 | 152.0 | 226610 | 250.0000 | ng | 0.003 |

System Monitoring Compounds

| | | | | | | |
|-------------------------|----------------------|-------|--------|--------------------|----|--------|
| S Dibromofluoromethane | 5.845 | 113.0 | 195966 | 277.6506 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 80.0 - 119.0% | | | Recovery = 111.06% | | |
| S 1,2-Dichloroethane-d4 | 6.230 | 67.0 | 88868 | 291.5091 | ng | -0.003 |
| Spiked Amount: 250.000 | Range: 81.0 - 118.0% | | | Recovery = 116.60% | | |
| S Toluene-d8 | 8.322 | 98.0 | 758617 | 267.0901 | ng | 0.003 |
| Spiked Amount: 250.000 | Range: 89.0 - 112.0% | | | Recovery = 106.84% | | |
| S p-Bromofluorobenzene | 10.948 | 95.0 | 219115 | 263.9340 | ng | -0.006 |
| Spiked Amount: 250.000 | Range: 85.0 - 114.0% | | | Recovery = 105.57% | | |

Target Compounds









| Compound | RT | QIon | Resp. | Conc. | Units | QValue |
|----------------------------------|-------|------|-------|--------|-------|--------|
| T Dichlorodifluoromethane | 0.000 | | 0 | N.D. | | |
| T Chloromethane | 0.000 | | 0 | N.D. | | |
| T Vinyl chloride | 0.000 | | 0 | N.D. | | |
| T Bromomethane | 0.000 | | 0 | N.D. | | |
| T Chloroethane | 0.000 | | 0 | N.D. | | |
| T Trichlorofluoromethane | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methylene chloride | 3.338 | 49.0 | 1656 | 1.4886 | ng | m 84 |
| T trans-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methyl tert-butyl ether (MTBE) | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloroethane | 0.000 | | 0 | N.D. | | |
| T 2,2-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T cis-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methyl ethyl ketone | 0.000 | | 0 | N.D. | | |
| T Bromochloromethane | 0.000 | | 0 | N.D. | | |
| T Chloroform | 0.000 | | 0 | N.D. | | |

Quantitation Results Report (QT Reviewed)

| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|-----------------------------|-------|------|-------|-------|-------|----------|
| T 1,1,1-Trichloroethane | 0.000 | | 0 | N.D. | | |
| T Carbon tetrachloride | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloropropene | 0.000 | | 0 | N.D. | | |
| T Benzene | 0.000 | | 0 | N.D. | | |
| T 1,2-Dichloroethane | 0.000 | | 0 | N.D. | | |
| T Trichloroethene | 0.000 | | 0 | N.D. | | |
| T 1,2-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T Dibromomethane | 0.000 | | 0 | N.D. | | |
| T Bromodichloromethane | 0.000 | | 0 | N.D. | | |
| T cis-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | |
| T Toluene | 0.000 | | 0 | N.D. | | |
| T trans-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | |
| T 1,1,2-Trichloroethane | 0.000 | | 0 | N.D. | | |
| T Tetrachloroethene | 0.000 | | 0 | N.D. | | |
| T 1,3-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T Chlorodibromomethane | 0.000 | | 0 | N.D. | | |
| T 1,2-Dibromoethane | 0.000 | | 0 | N.D. | | |
| T Chlorobenzene | 0.000 | | 0 | N.D. | | |
| T 1,1,1,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | |
| T Ethylbenzene | 0.000 | | 0 | N.D. | | |
| T m+p-Xylenes | 0.000 | | 0 | N.D. | | |
| T o-Xylene | 0.000 | | 0 | N.D. | | |
| T Styrene | 0.000 | | 0 | N.D. | | |
| T Bromoform | 0.000 | | 0 | N.D. | | |
| T Bromobenzene | 0.000 | | 0 | N.D. | | |
| T 1,1,2,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | |
| T 1,2,3-Trichloropropane | 0.000 | | 0 | N.D. | | |
| T 2-Chlorotoluene | 0.000 | | 0 | N.D. | | |
| T 4-Chlorotoluene | 0.000 | | 0 | N.D. | | |
| T 1,3-Dichlorobenzene | 0.000 | | 0 | N.D. | | |
| T 1,4-Dichlorobenzene | 0.000 | | 0 | N.D. | | |
| T 1,2-Dichlorobenzene | 0.000 | | 0 | N.D. | | |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)

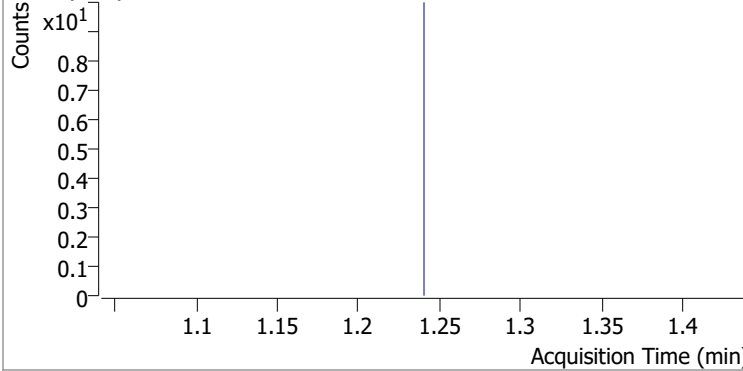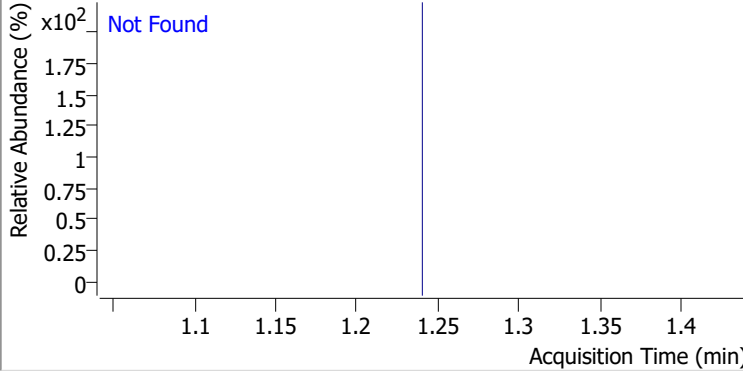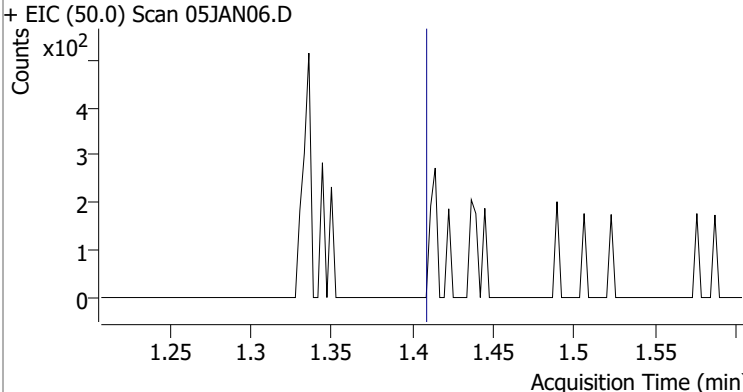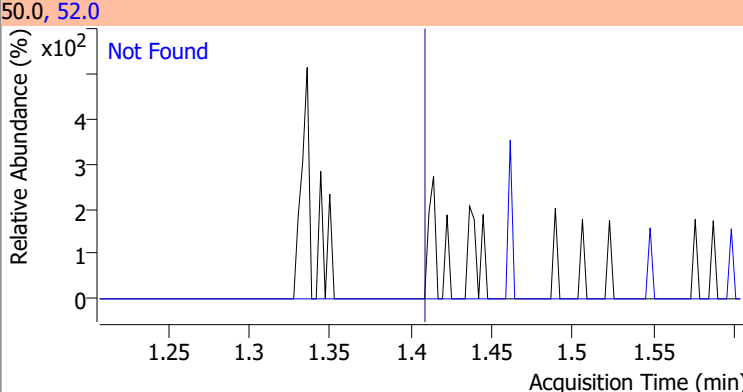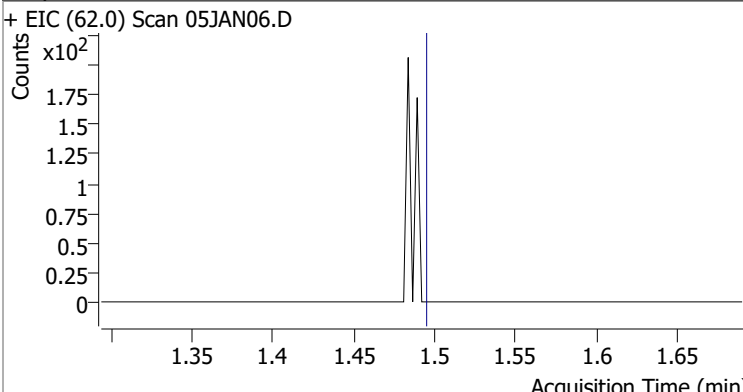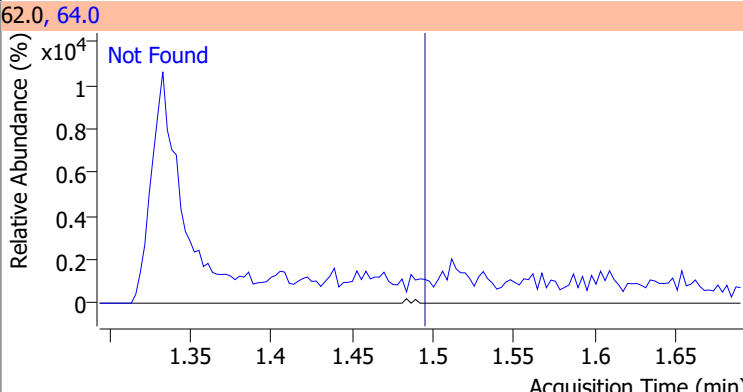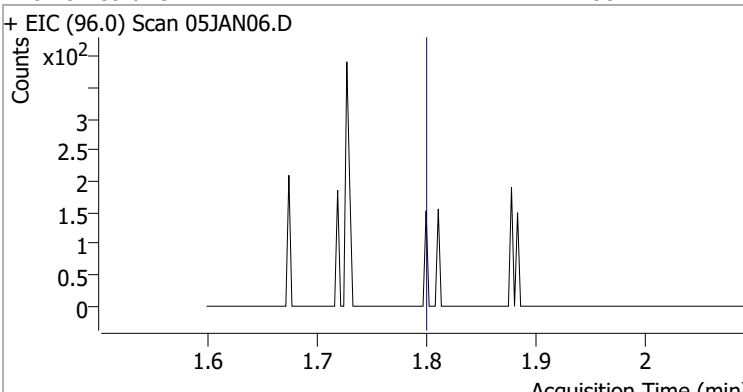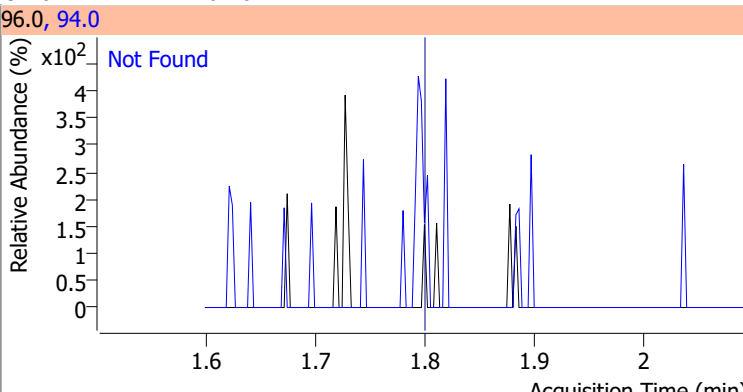
| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--|-------|--------|--|-----------|
| Dichlorodifluoromethane | N.D. | 1.24 | 87.0 | 32.3 |
| + EIC (85.0) Scan 05JAN06.D ***NO DATA POINTS*** | | | 85.0, 87.0 | |
|  | | |  | |
| Chloromethane | N.D. | 1.41 | 52.0 | 32.1 |
| + EIC (50.0) Scan 05JAN06.D | | | 50.0, 52.0 | |
|  | | |  | |
| Vinyl chloride | N.D. | 1.50 | 64.0 | 29.9 |
| + EIC (62.0) Scan 05JAN06.D | | | 62.0, 64.0 | |
|  | | |  | |
| Bromomethane | N.D. | 1.80 | 94.0 | 104.6 |
| + EIC (96.0) Scan 05JAN06.D | | | 96.0, 94.0 | |
|  | | |  | |

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------|-------|--------|------|-----------|
| Chloroethane | N.D. | 1.89 | 66.0 | 30.1 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|------------------------|-------|--------|-------|-----------|
| Trichlorofluoromethane | N.D. | 2.14 | 103.0 | 64.2 |











| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethene | N.D. | 2.70 | 61.0 | 180.3 | 63.0 | 56.7 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|--------|------|----------|----------|------|--------|-------|-------|
| Methylene chloride | 1.4886 | 3.34 | 0.00 | 1656 (m) | 84.0 | 47.3 | 36.9 | 96.9 |
| | | | | | 86.0 | 46.1 | 14.3 | 74.3 |




Quantitation Results Report (QT Reviewed)

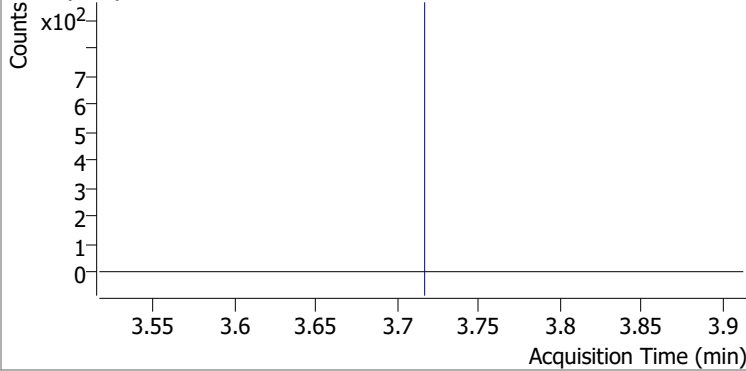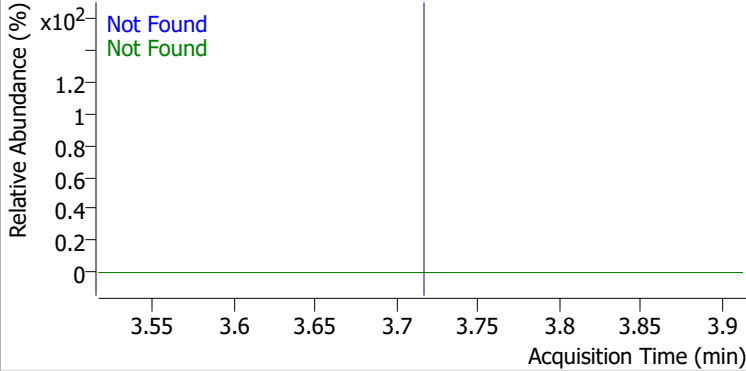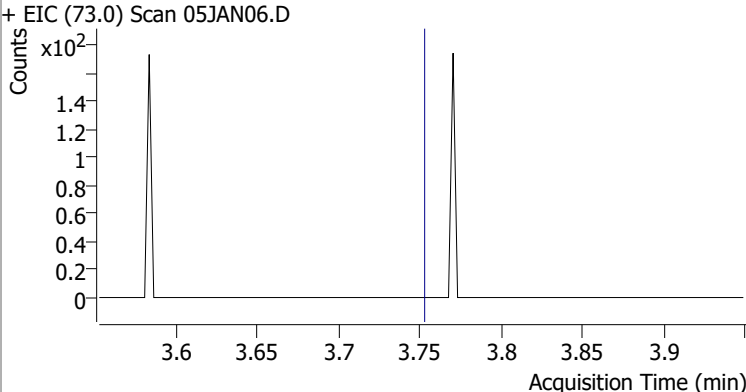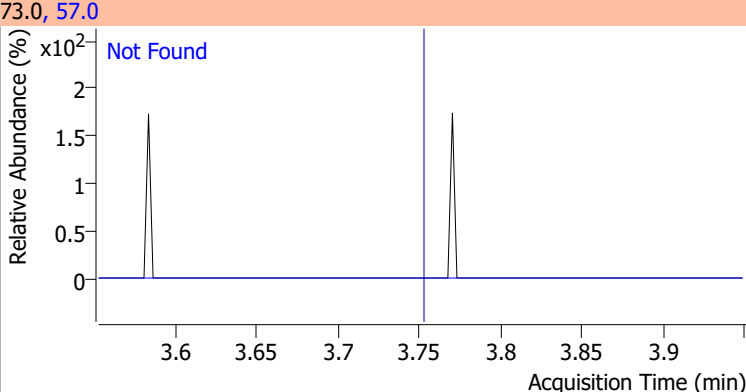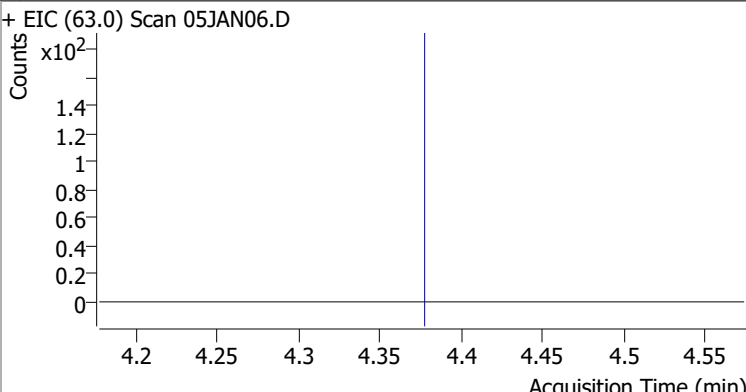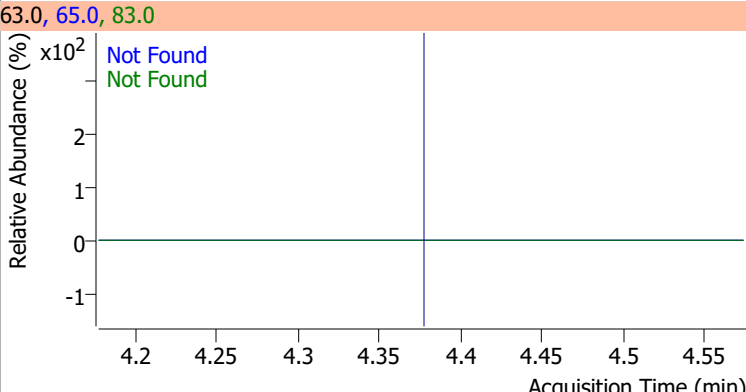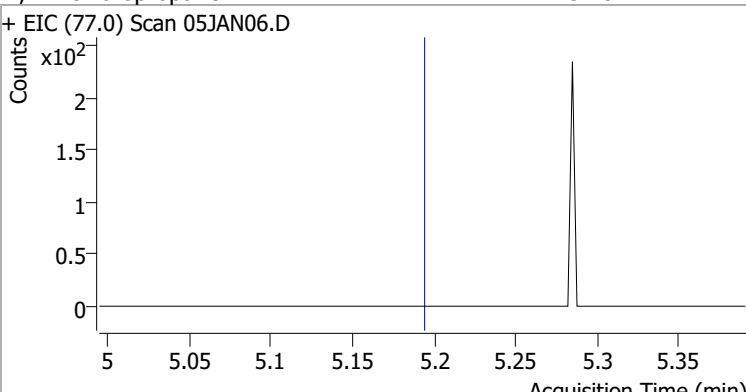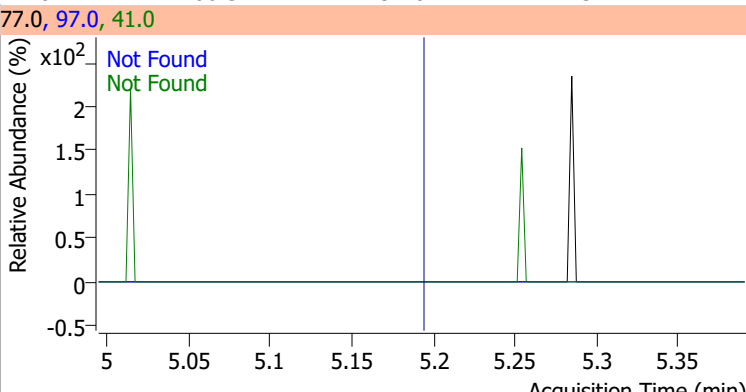
| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--|-------|--------|--|-----------|------|-----------|
| trans-1,2-Dichloroethene | N.D. | 3.72 | 61.0 | 153.9 | 98.0 | 65.7 |
| + EIC (96.0) Scan 05JAN06.D | | | 96.0, 61.0, 98.0 | | | |
|  | | |  | | | |
| Methyl tert-butyl ether (MTBE) | N.D. | 3.75 | 57.0 | 24.6 | | |
| + EIC (73.0) Scan 05JAN06.D | | | 73.0, 57.0 | | | |
|  | | |  | | | |
| 1,1-Dichloroethane | N.D. | 4.38 | 65.0 | 32.1 | 83.0 | 13.7 |
| + EIC (63.0) Scan 05JAN06.D | | | 63.0, 65.0, 83.0 | | | |
|  | | |  | | | |
| 2,2-Dichloropropane | N.D. | 5.20 | 41.0 | 66.5 | 97.0 | 23.2 |
| + EIC (77.0) Scan 05JAN06.D | | | 77.0, 97.0, 41.0 | | | |
|  | | |  | | | |

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|------------------------|-------|--------|------|-----------|------|-----------|
| cis-1,2-Dichloroethene | N.D. | 5.22 | 61.0 | 167.2 | 98.0 | 67.3 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| Methyl ethyl ketone | N.D. | 5.28 | 72.0 | 21.3 |







| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|
| Bromochloromethane | N.D. | 5.52 | 49.0 | 182.9 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|------------|-------|--------|------|-----------|
| Chloroform | N.D. | 5.65 | 85.0 | 66.0 |




Quantitation Results Report (QT Reviewed)

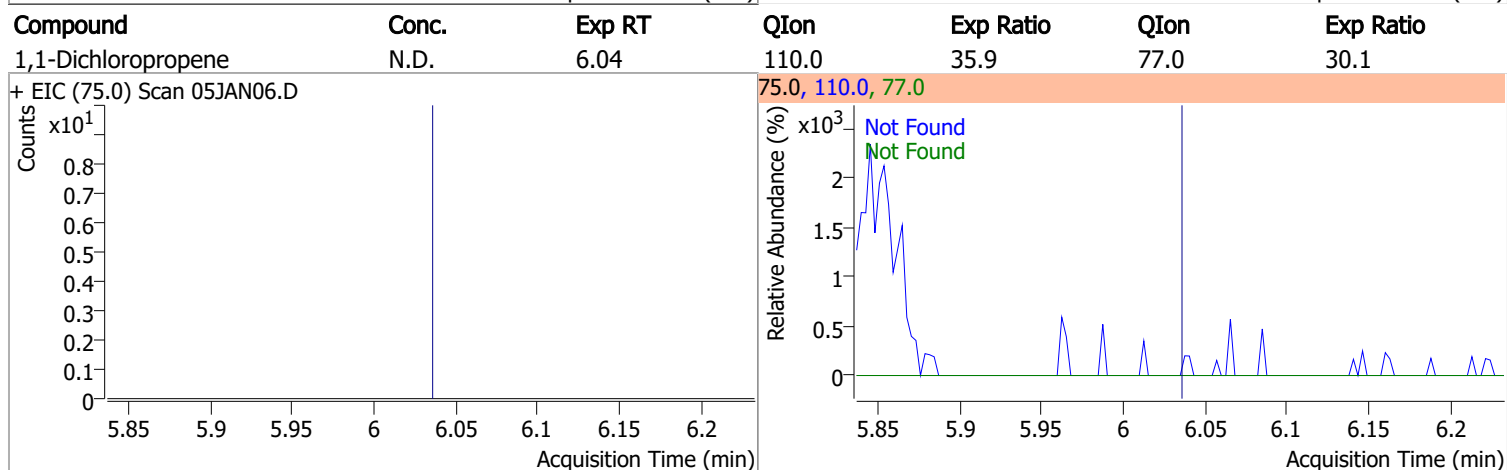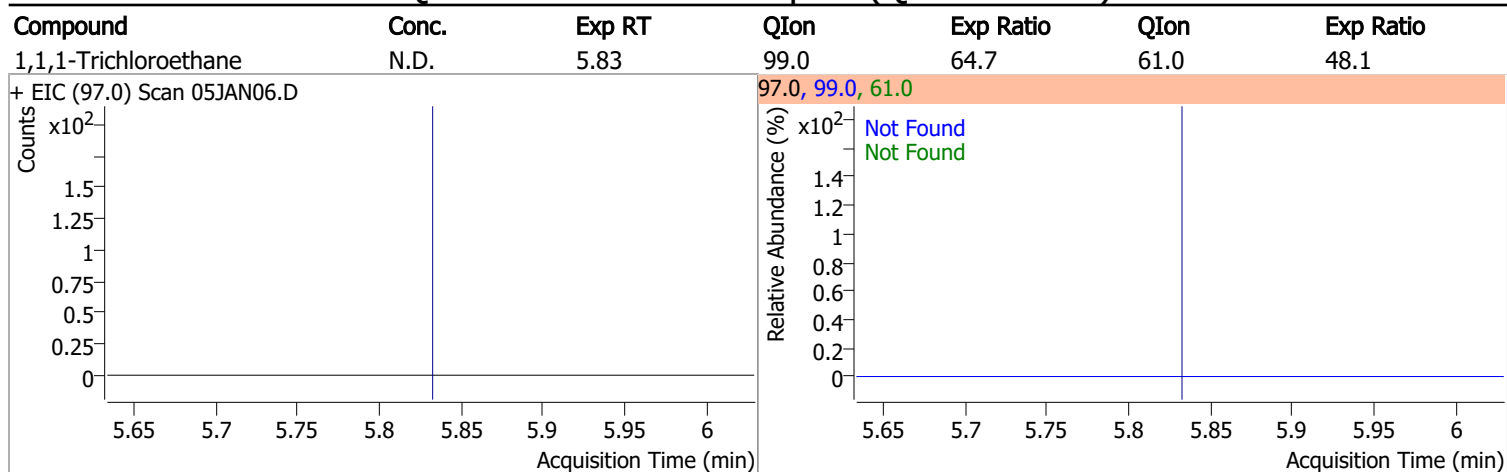


Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 291.5091 | 6.23 | 0.00 | 88868 | 65.0 | 192.8 | 166.5 | 226.5 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------|-------|--------|------|-----------|
| Benzene | N.D. | 6.28 | 77.0 | 23.5 |







| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,2-Dichloroethane | N.D. | 6.32 | 64.0 | 29.9 | 98.0 | 7.6 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------|-------|--------|-------|-----------|------|-----------|
| Trichloroethene | N.D. | 7.03 | 130.0 | 101.5 | 97.0 | 64.1 |




Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 267.0901 | 8.32 | 0.00 | 758617 | 100.0 | 63.1 | 34.4 | 94.4 |
| | | | | | 99.0 | 9.5 | 0.0 | 39.6 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------|-------|--------|------|-----------|
| Toluene | N.D. | 8.39 | 91.0 | 175.8 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,3-Dichloropropene | N.D. | 8.64 | 39.0 | 53.4 | 77.0 | 32.4 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------------|-------|--------|------|-----------|------|-----------|
| 1,1,2-Trichloroethane | N.D. | 8.82 | 97.0 | 114.6 | 85.0 | 67.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-------------------|-------|--------|-------|-----------|-------|-----------|
| Tetrachloroethene | N.D. | 8.94 | 165.8 | 128.6 | 129.0 | 91.5 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| 1,3-Dichloropropane | N.D. | 8.98 | 78.0 | 32.9 |







| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------------------|-------|--------|-------|-----------|
| Chlorodibromomethane | N.D. | 9.21 | 127.0 | 78.0 |






| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|-------------------|-------|--------|-------|-----------|
| 1,2-Dibromoethane | N.D. | 9.31 | 109.0 | 94.5 |




Quantitation Results Report (QT Reviewed)

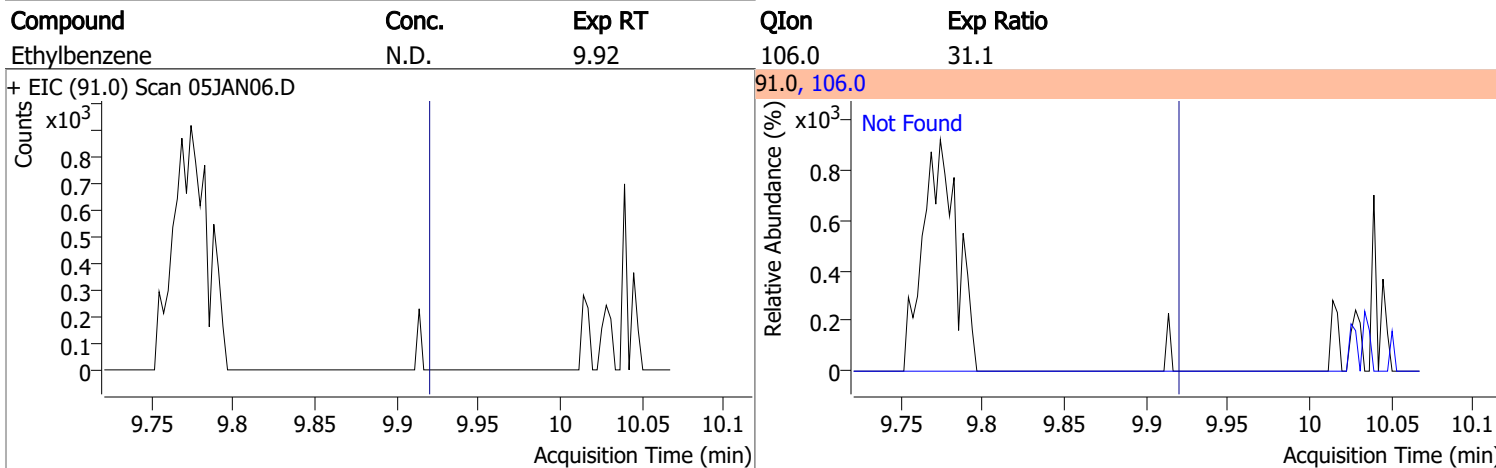









Quantitation Results Report (QT Reviewed)

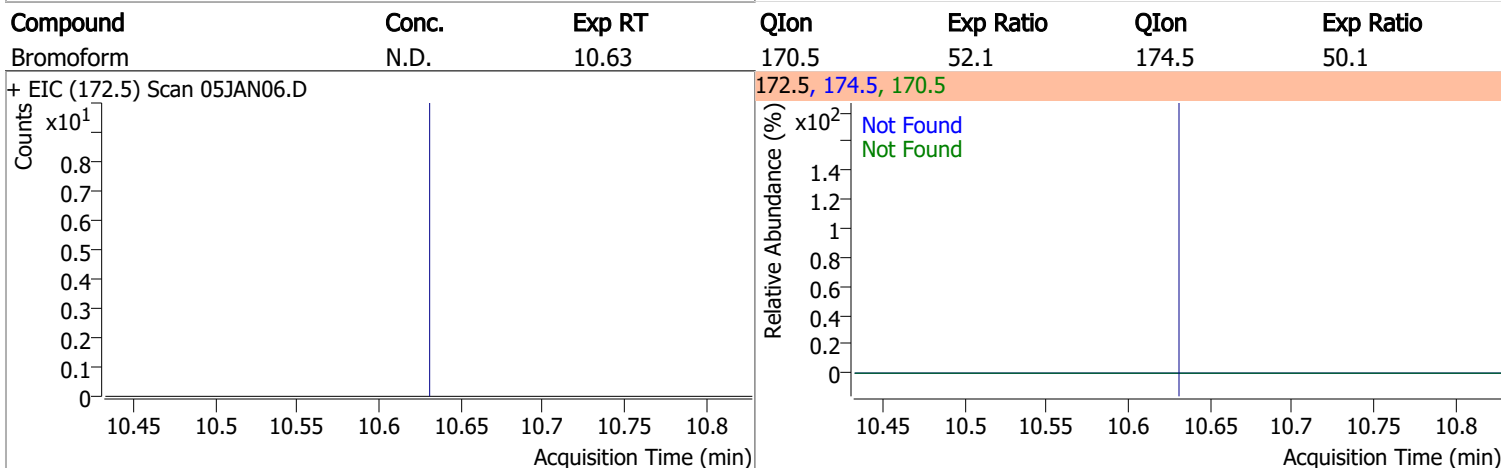





| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 263.9340 | 10.95 | -0.01 | 219115 | 174.0 | 96.5 | 61.7 | 121.7 |
| | | | | | 176.0 | 92.6 | 60.6 | 120.6 |



Quantitation Results Report (QT Reviewed)

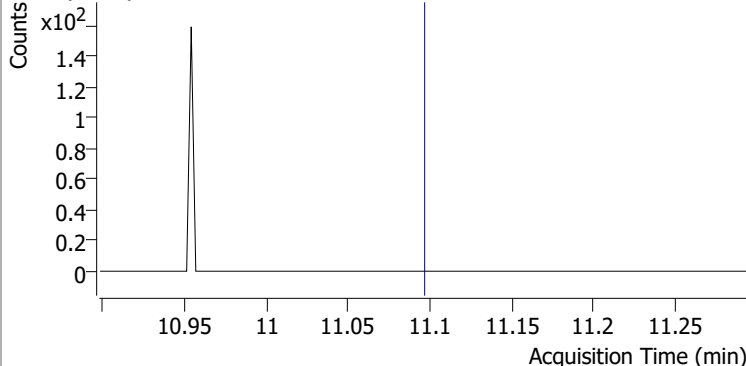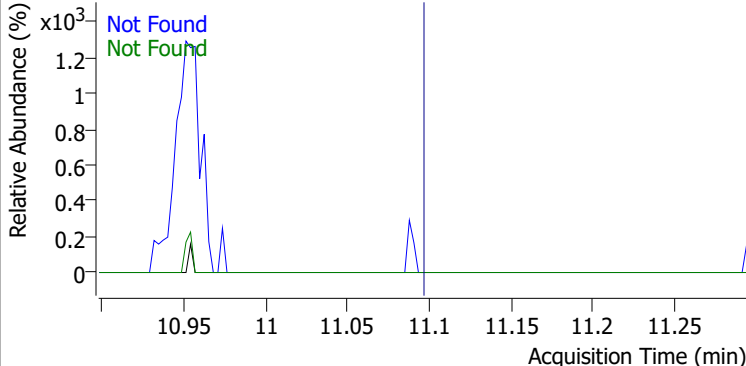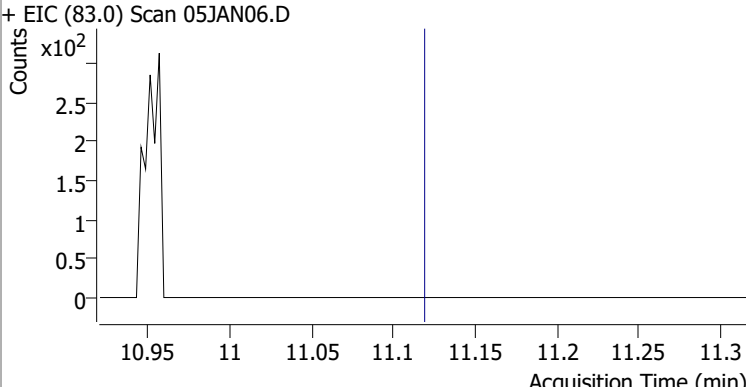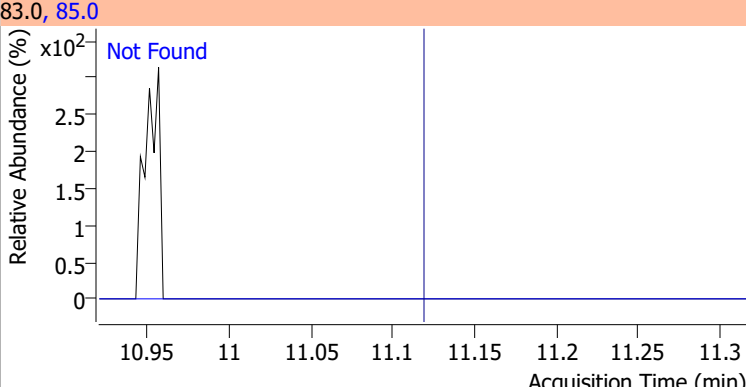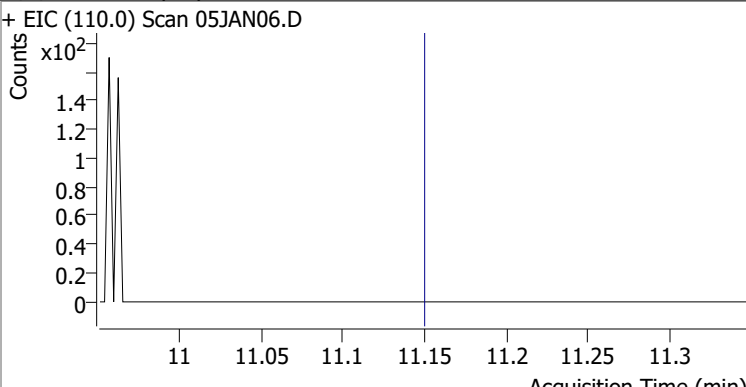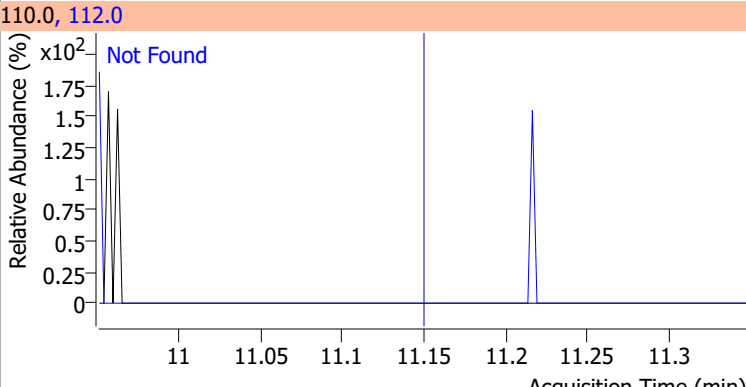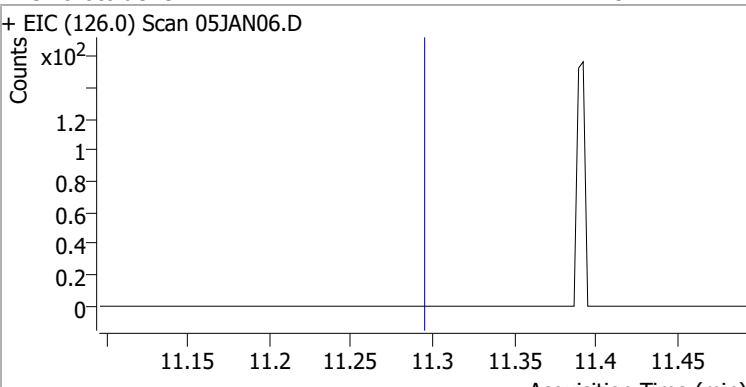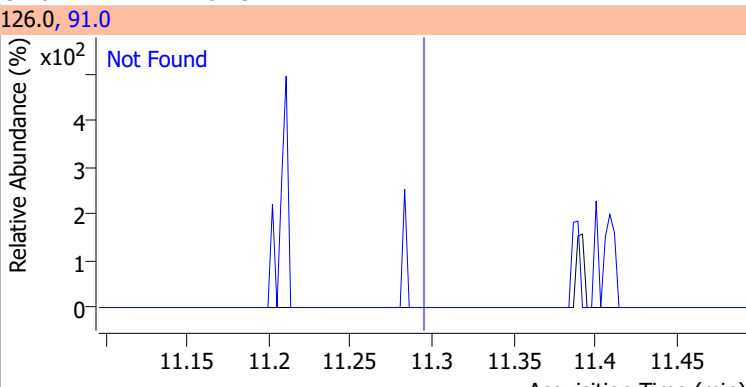
| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--|-------|--------|--|-----------|-------|-----------|
| Bromobenzene | N.D. | 11.09 | 77.0 | 145.7 | 158.0 | 96.5 |
| + EIC (156.0) Scan 05JAN06.D | | | 156.0, 77.0, 158.0 | | | |
|  | | |  | | | |
| 1,1,2,2-Tetrachloroethane | N.D. | 11.12 | 85.0 | 66.2 | | |
| + EIC (83.0) Scan 05JAN06.D | | | 83.0, 85.0 | | | |
|  | | |  | | | |
| 1,2,3-Trichloropropane | N.D. | 11.15 | 112.0 | 63.5 | | |
| + EIC (110.0) Scan 05JAN06.D | | | 110.0, 112.0 | | | |
|  | | |  | | | |
| 2-Chlorotoluene | N.D. | 11.29 | 91.0 | 282.3 | | |
| + EIC (126.0) Scan 05JAN06.D | | | 126.0, 91.0 | | | |
|  | | |  | | | |

Quantitation Results Report (QT Reviewed)

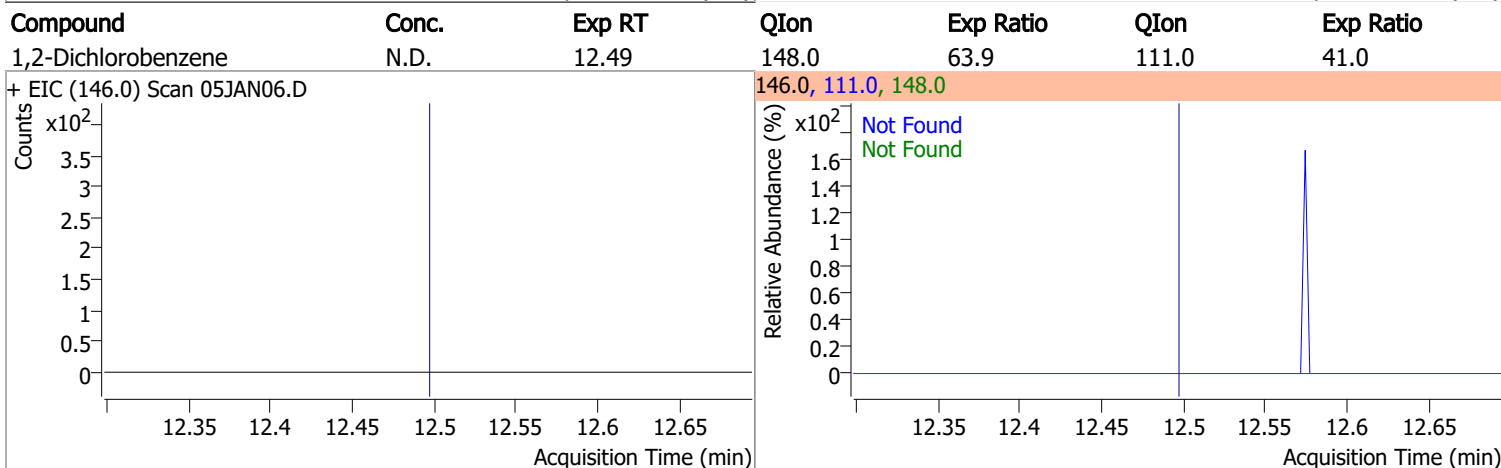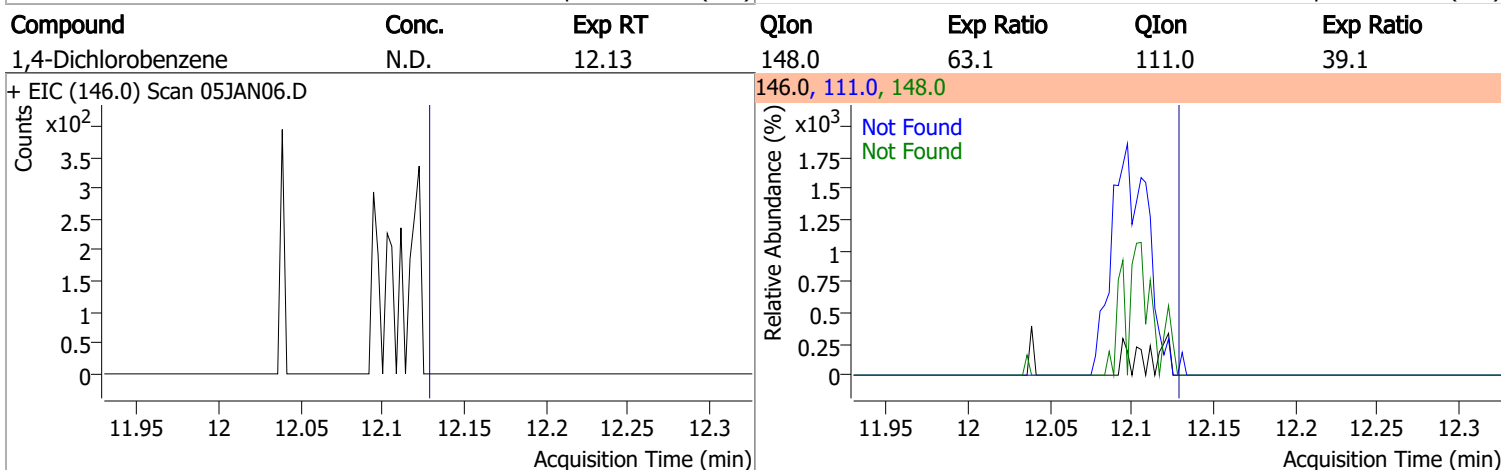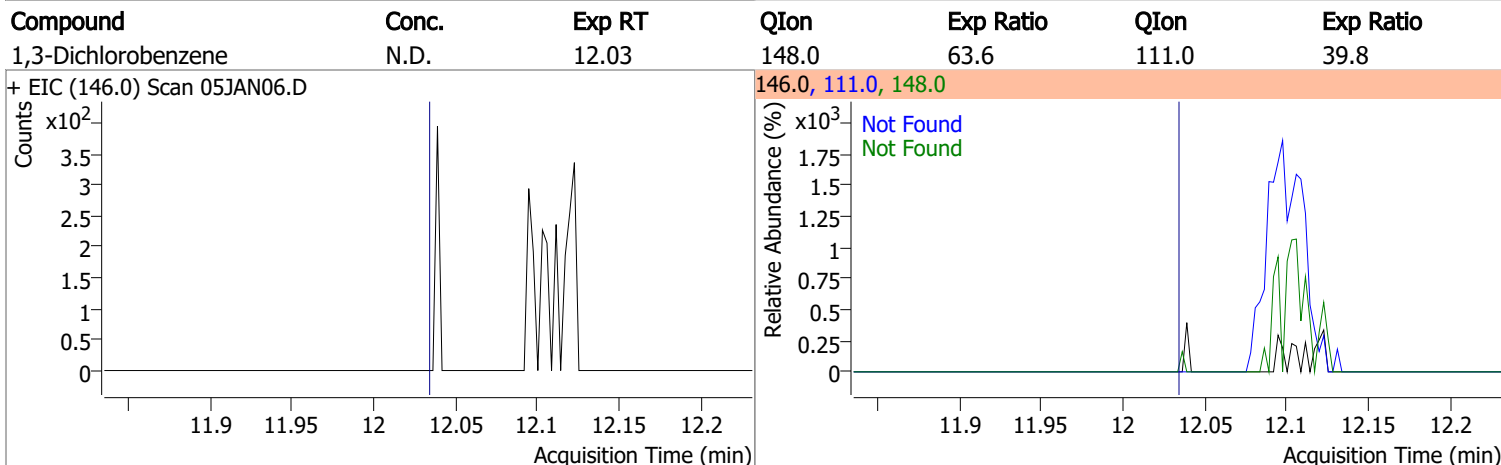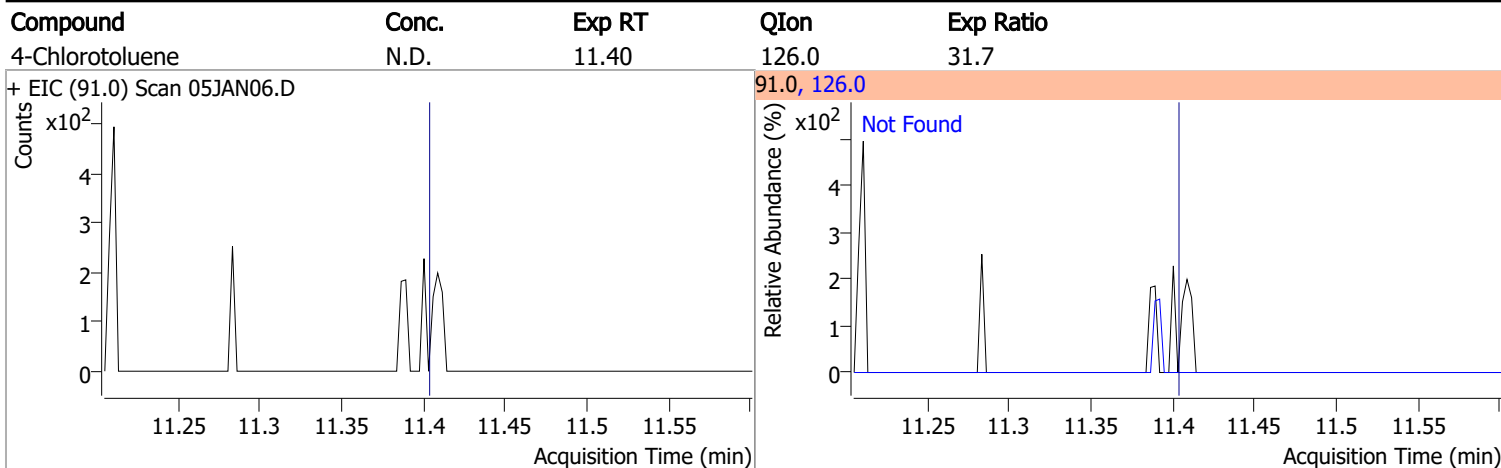

Quantitation Results Report (QT Reviewed)

| | | | |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File | 05JAN07.D | Operator | MSC |
| Acq. Method | 5975CACQF.M | Acq. Date-Time | 1/5/2022 12:49:15 PM |
| Sample Name | B22010002-004A | Instrument | VOA5975C |
| Vial | 7 | Multiplier | 1.00 |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m | Comment | |
| Tune File | BFB_Atune3.u | Tune Date | 10/11/2021 4:02:00 PM |
| Batch Name | VG010522_8260B.batch.bin | Last Calib Update | 2/28/2022 2:48:47 PM |
| Ref Library | \\MASSHUNTER\Org\Library\NIST129K.I | | |







| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|----------------------|-------|----------|
| Internal Standards | | | | | | |
| M Fluorobenzene | 6.620 | 96.0 | 690751 | 250.0000 | ng | -0.003 |
| M Chlorobenzene-d5 | 9.774 | 82.0 | 266290 | 250.0000 | ng | 0.003 |
| M 1,4-Dichlorobenzene-d4 | 12.100 | 152.0 | 193287 | 250.0000 | ng | 0.000 |
| System Monitoring Compounds | | | | | | |
| S Dibromofluoromethane | 5.848 | 113.0 | 182638 | 280.6545 | ng | 0.003 |
| Spiked Amount: 250.000 | Range: 80.0 - 119.0% | | | Recovery = 112.26% | | |
| S 1,2-Dichloroethane-d4 | 6.233 | 67.0 | 83829 | 298.2386 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 81.0 - 118.0% | | | Recovery = 119.30% * | | |
| S Toluene-d8 | 8.319 | 98.0 | 684900 | 266.9024 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 89.0 - 112.0% | | | Recovery = 106.76% | | |
| S p-Bromofluorobenzene | 10.951 | 95.0 | 199881 | 282.2742 | ng | -0.003 |
| Spiked Amount: 250.000 | Range: 85.0 - 114.0% | | | Recovery = 112.91% | | |
| Target Compounds | | | | | | |
| T Dichlorodifluoromethane | 0.000 | | 0 | N.D. | | |
| T Chloromethane | 1.411 | 50.0 | 579 | 0.5270 | ng | m 62 |
| T Vinyl chloride | 0.000 | | 0 | N.D. | | |
| T Bromomethane | 0.000 | | 0 | N.D. | | |
| T Chloroethane | 0.000 | | 0 | N.D. | | |
| T Trichlorofluoromethane | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methylene chloride | 3.338 | 49.0 | 1563 | 1.5237 | ng | m 81 |
| T trans-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methyl tert-butyl ether (MTBE) | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloroethane | 0.000 | | 0 | N.D. | | |
| T 2,2-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T cis-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methyl ethyl ketone | 0.000 | | 0 | N.D. | | |
| T Bromochloromethane | 0.000 | | 0 | N.D. | | |
| T Chloroform | 0.000 | | 0 | N.D. | | |

Quantitation Results Report (QT Reviewed)




| Compound | RT | QIon | Resp. | Conc. | Units | | Dev(Min) |
|-----------------------------|-------|------|-------|--------|-------|---|----------|
| T 1,1,1-Trichloroethane | 0.000 | | 0 | N.D. | | | |
| T Carbon tetrachloride | 0.000 | | 0 | N.D. | | | |
| T 1,1-Dichloropropene | 0.000 | | 0 | N.D. | | | |
| T Benzene | 6.277 | 78.0 | 306 | 0.1114 | ng | m | 89 |
| T 1,2-Dichloroethane | 0.000 | | 0 | N.D. | | | |
| T Trichloroethene | 0.000 | | 0 | N.D. | | | |
| T 1,2-Dichloropropane | 0.000 | | 0 | N.D. | | | |
| T Dibromomethane | 0.000 | | 0 | N.D. | | | |
| T Bromodichloromethane | 0.000 | | 0 | N.D. | | | |
| T cis-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | | |
| T Toluene | 8.386 | 92.0 | 1710 | 0.9866 | ng | m | 98 |
| T trans-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | | |
| T 1,1,2-Trichloroethane | 0.000 | | 0 | N.D. | | | |
| T Tetrachloroethene | 0.000 | | 0 | N.D. | | | |
| T 1,3-Dichloropropane | 0.000 | | 0 | N.D. | | | |
| T Chlorodibromomethane | 0.000 | | 0 | N.D. | | | |
| T 1,2-Dibromoethane | 0.000 | | 0 | N.D. | | | |
| T Chlorobenzene | 0.000 | | 0 | N.D. | | | |
| T 1,1,1,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | | |
| T Ethylbenzene | 0.000 | | 0 | N.D. | | | |
| T m+p-Xylenes | 0.000 | | 0 | N.D. | | | |
| T o-Xylene | 0.000 | | 0 | N.D. | | | |
| T Styrene | 0.000 | | 0 | N.D. | | | |
| T Bromoform | 0.000 | | 0 | N.D. | | | |
| T Bromobenzene | 0.000 | | 0 | N.D. | | | |
| T 1,1,2,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | | |
| T 1,2,3-Trichloropropane | 0.000 | | 0 | N.D. | | | |
| T 2-Chlorotoluene | 0.000 | | 0 | N.D. | | | |
| T 4-Chlorotoluene | 0.000 | | 0 | N.D. | | | |
| T 1,3-Dichlorobenzene | 0.000 | | 0 | N.D. | | | |
| T 1,4-Dichlorobenzene | 0.000 | | 0 | N.D. | | | |
| T 1,2-Dichlorobenzene | 0.000 | | 0 | N.D. | | | |

(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak


Quantitation Results Report (QT Reviewed)



Quantitation Results Report (QT Reviewed)




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|--------|------|----------|----------|------|--------|-------|-------|
| Methylene chloride | 1.5237 | 3.34 | 0.00 | 1563 (m) | 84.0 | 60.8 | 36.9 | 96.9 |
| | | | | | 86.0 | 20.2 | 14.3 | 74.3 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,2-Dichloroethene | N.D. | 3.72 | 61.0 | 153.9 | 98.0 | 65.7 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------------------|-------|--------|------|-----------|
| Methyl tert-butyl ether (MTBE) | N.D. | 3.75 | 57.0 | 24.6 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethane | N.D. | 4.38 | 65.0 | 32.1 | 83.0 | 13.7 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|------|-----------|
| 2,2-Dichloropropane | N.D. | 5.20 | 41.0 | 66.5 | 97.0 | 23.2 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|------------------------|-------|--------|------|-----------|------|-----------|
| cis-1,2-Dichloroethene | N.D. | 5.22 | 61.0 | 167.2 | 98.0 | 67.3 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| Methyl ethyl ketone | N.D. | 5.28 | 72.0 | 21.3 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|
| Bromochloromethane | N.D. | 5.52 | 49.0 | 182.9 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|------------|-------|--------|------|-----------|
| Chloroform | N.D. | 5.65 | 85.0 | 66.0 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------------|-------|--------|------|-----------|------|-----------|
| 1,1,1-Trichloroethane | N.D. | 5.83 | 99.0 | 64.7 | 61.0 | 48.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Dibromofluoromethane | 280.6545 | 5.85 | 0.00 | 182638 | 191.5 | 22.0 | 0.0 | 53.1 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|----------------------|-------|--------|-------|-----------|-------|-----------|
| Carbon tetrachloride | N.D. | 6.02 | 119.0 | 97.2 | 121.0 | 30.1 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|-------|-----------|------|-----------|
| 1,1-Dichloropropene | N.D. | 6.04 | 110.0 | 35.9 | 77.0 | 30.1 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 298.2386 | 6.23 | 0.00 | 83829 | 65.0 | 195.5 | 166.5 | 226.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|--------|------|----------|---------|------|--------|-------|-------|
| Benzene | 0.1114 | 6.28 | 0.00 | 306 (m) | 77.0 | 18.2 | 0.0 | 53.5 |











| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,2-Dichloroethane | N.D. | 6.32 | 64.0 | 29.9 | 98.0 | 7.6 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------|-------|--------|-------|-----------|------|-----------|
| Trichloroethene | N.D. | 7.03 | 130.0 | 101.5 | 97.0 | 64.1 |




Quantitation Results Report (QT Reviewed)

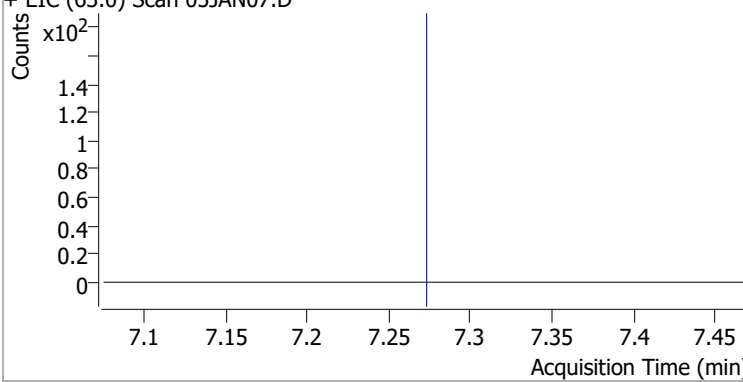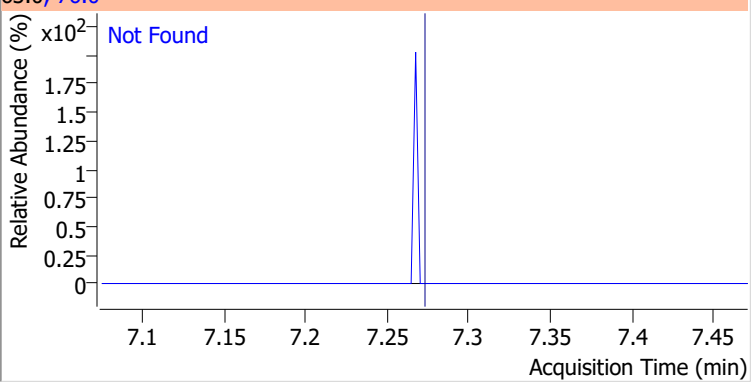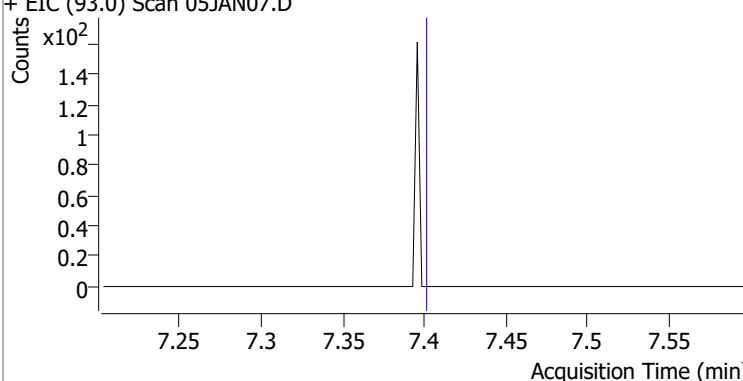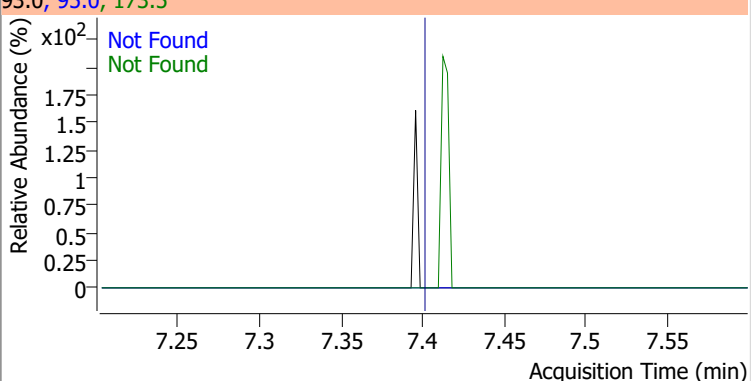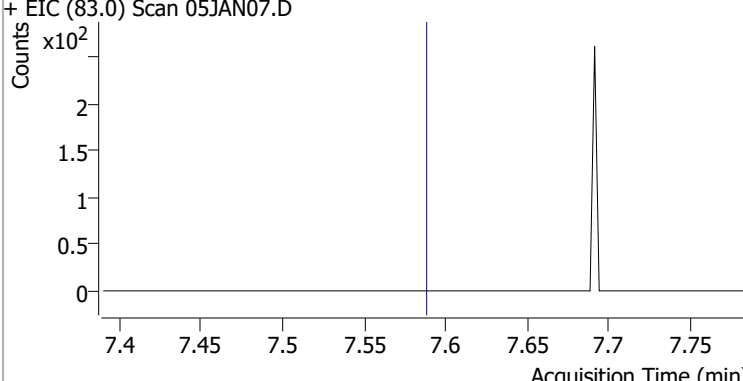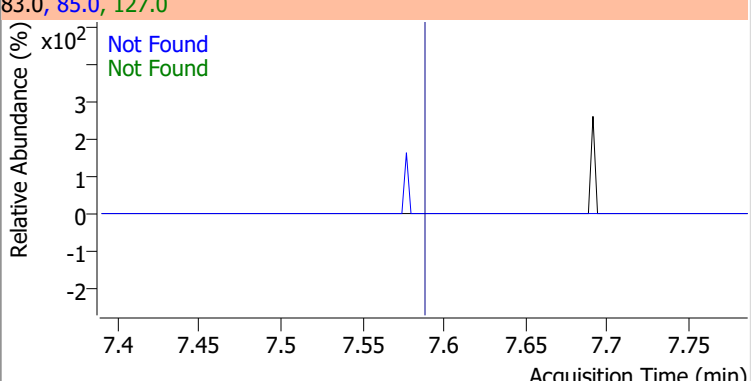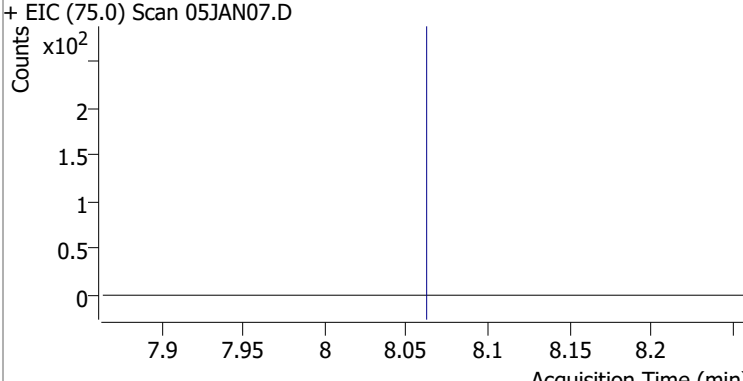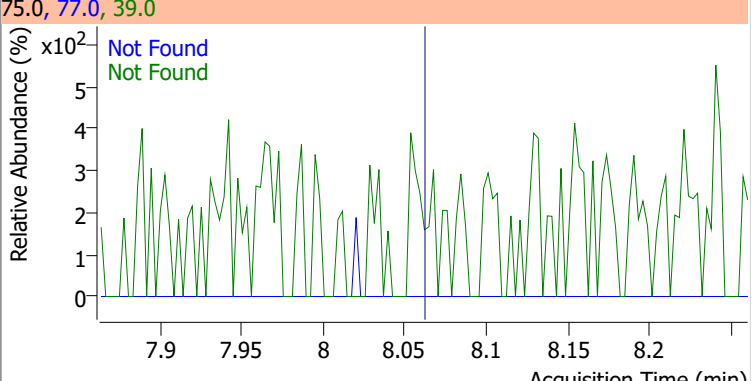
| Compound | Conc. | Exp RT | QIon | Exp Ratio | | |
|--|-------|--------|--|-----------|------|-----------|
| 1,2-Dichloropropane | N.D. | 7.27 | 76.0 | 38.2 | | |
| + EIC (63.0) Scan 05JAN07.D | | | 63.0, 76.0 | | | |
|  | | |  | | | |
| Dibromomethane | N.D. | 7.40 | 173.5 | 113.7 | QIon | Exp Ratio |
| + EIC (93.0) Scan 05JAN07.D | | | 93.0, 95.0, 173.5 | | | |
|  | | |  | | | |
| Bromodichloromethane | N.D. | 7.59 | 85.0 | 64.5 | QIon | Exp Ratio |
| + EIC (83.0) Scan 05JAN07.D | | | 83.0, 85.0, 127.0 | | | |
|  | | |  | | | |
| cis-1,3-Dichloropropene | N.D. | 8.06 | 39.0 | 53.3 | QIon | Exp Ratio |
| + EIC (75.0) Scan 05JAN07.D | | | 75.0, 77.0, 39.0 | | | |
|  | | |  | | | |

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 266.9024 | 8.32 | 0.00 | 684900 | 100.0 | 63.0 | 34.4 | 94.4 |
| | | | | | 99.0 | 9.7 | 0.0 | 39.6 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|--------|------|----------|----------|------|--------|-------|-------|
| Toluene | 0.9866 | 8.39 | 0.00 | 1710 (m) | 91.0 | 178.5 | 145.8 | 205.8 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,3-Dichloropropene | N.D. | 8.64 | 39.0 | 53.4 | 77.0 | 32.4 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------------|-------|--------|------|-----------|------|-----------|
| 1,1,2-Trichloroethane | N.D. | 8.82 | 97.0 | 114.6 | 85.0 | 67.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-------------------|-------|--------|-------|-----------|-------|-----------|
| Tetrachloroethene | N.D. | 8.94 | 165.8 | 128.6 | 129.0 | 91.5 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| 1,3-Dichloropropane | N.D. | 8.98 | 78.0 | 32.9 |











| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------------------|-------|--------|-------|-----------|
| Chlorodibromomethane | N.D. | 9.21 | 127.0 | 78.0 |






| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|-------------------|-------|--------|-------|-----------|
| 1,2-Dibromoethane | N.D. | 9.31 | 109.0 | 94.5 |




Quantitation Results Report (QT Reviewed)
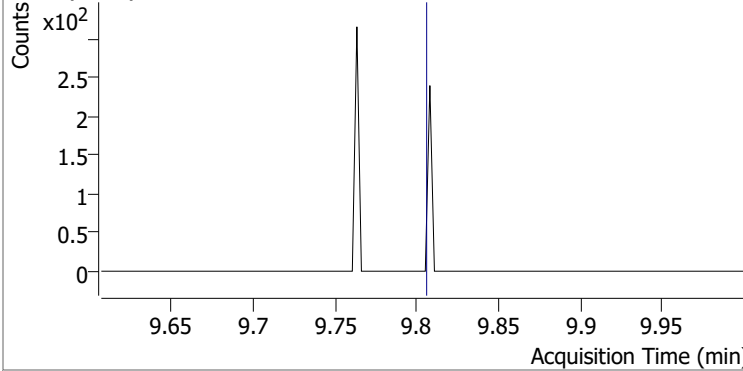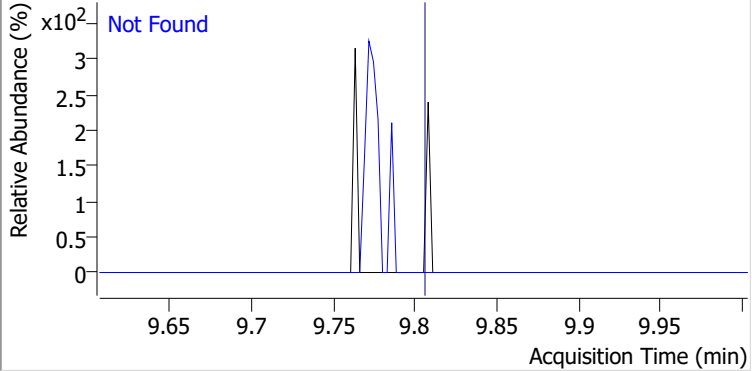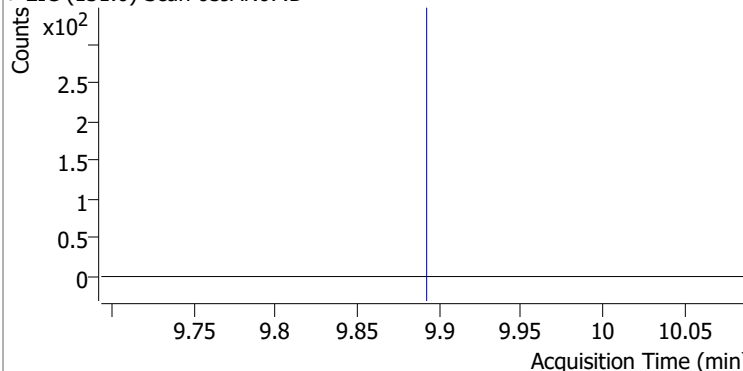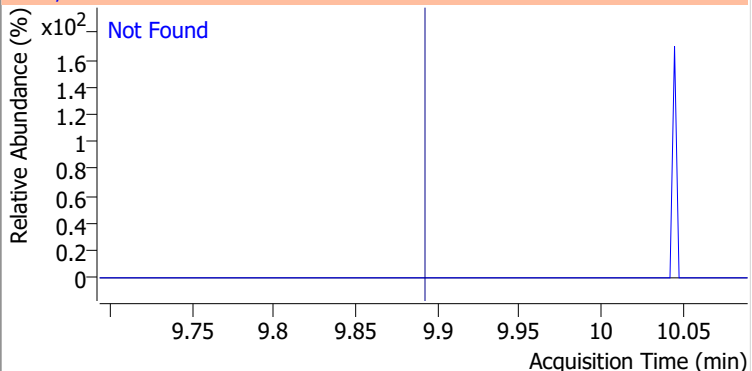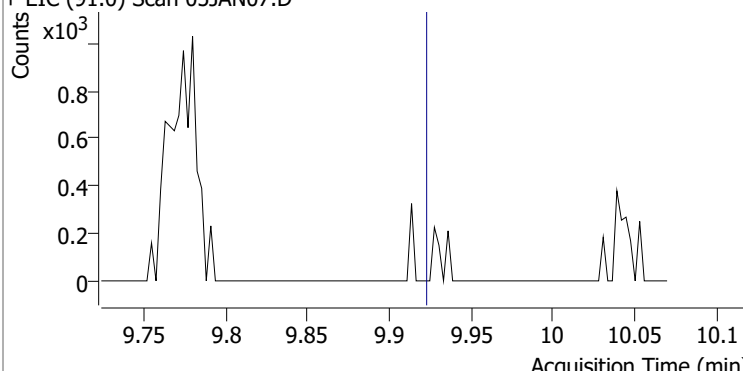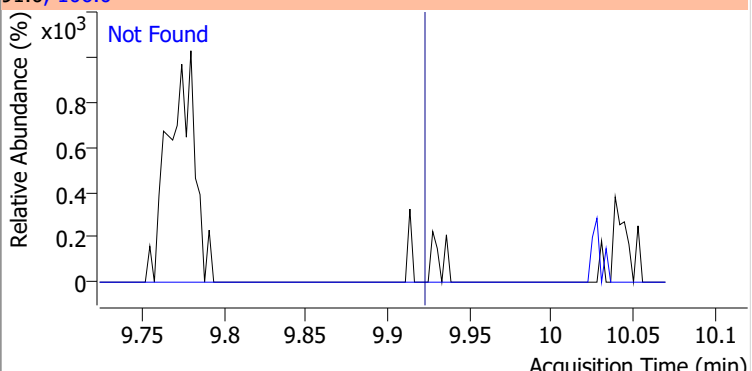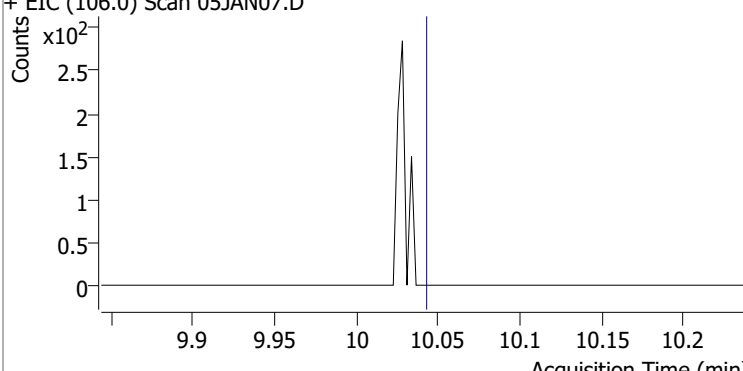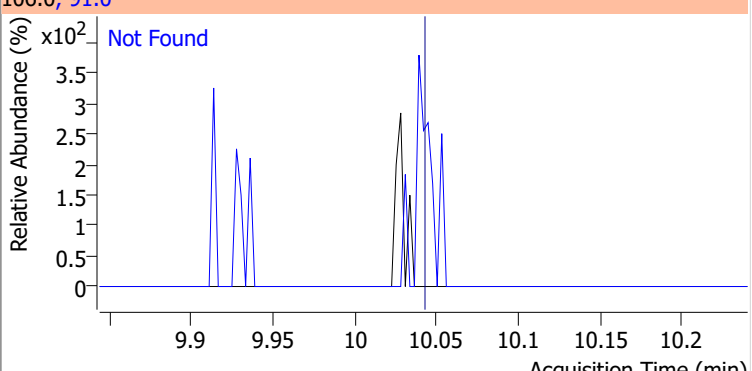
| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--|-------|--------|--|-----------|
| Chlorobenzene | N.D. | 9.80 | 114.0 | 32.1 |
| + EIC (112.0) Scan 05JAN07.D | | | 112.0, 114.0 | |
|  | | |  | |
| 1,1,1,2-Tetrachloroethane | N.D. | 9.89 | 133.0 | 98.6 |
| + EIC (131.0) Scan 05JAN07.D | | | 131.0, 133.0 | |
|  | | |  | |
| Ethylbenzene | N.D. | 9.92 | 106.0 | 31.1 |
| + EIC (91.0) Scan 05JAN07.D | | | 91.0, 106.0 | |
|  | | |  | |
| m+p-Xylenes | N.D. | 10.04 | 91.0 | 201.4 |
| + EIC (106.0) Scan 05JAN07.D | | | 106.0, 91.0 | |
|  | | |  | |









Quantitation Results Report (QT Reviewed)

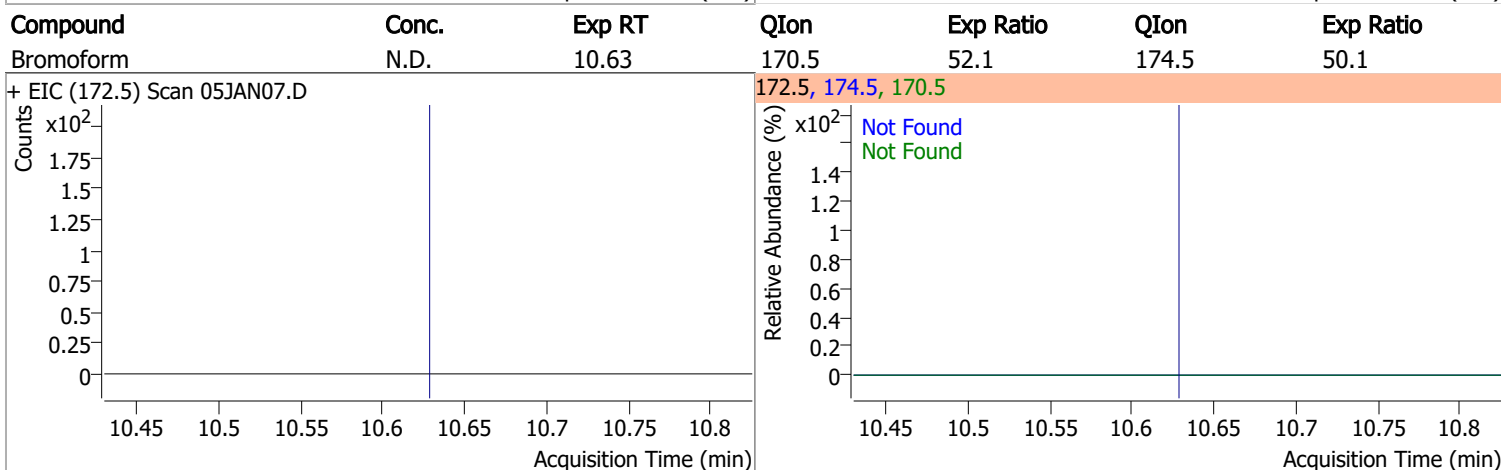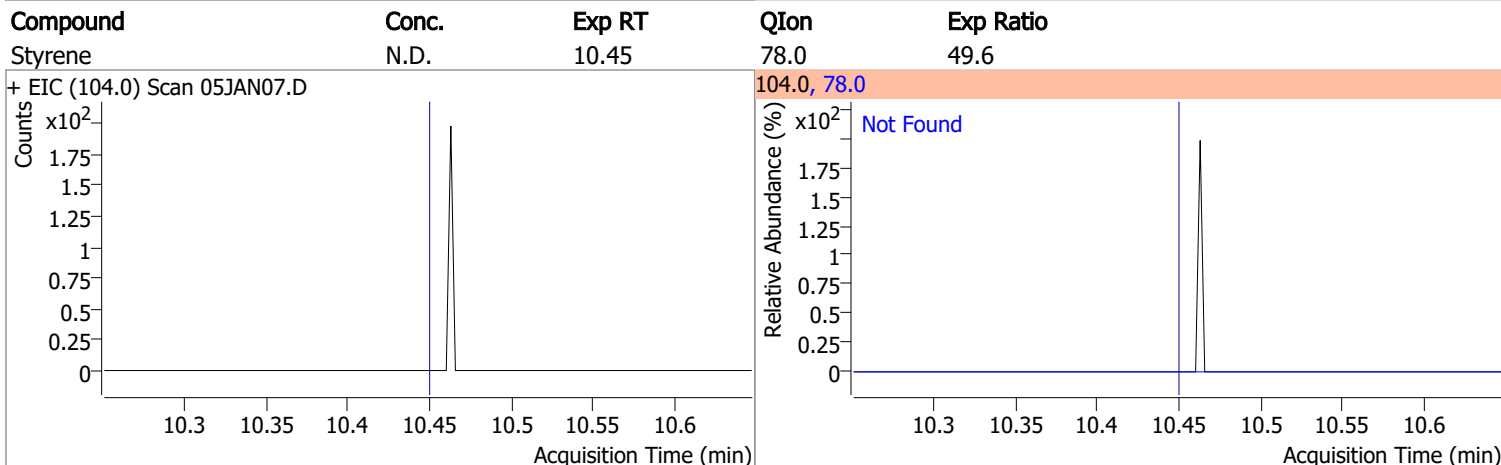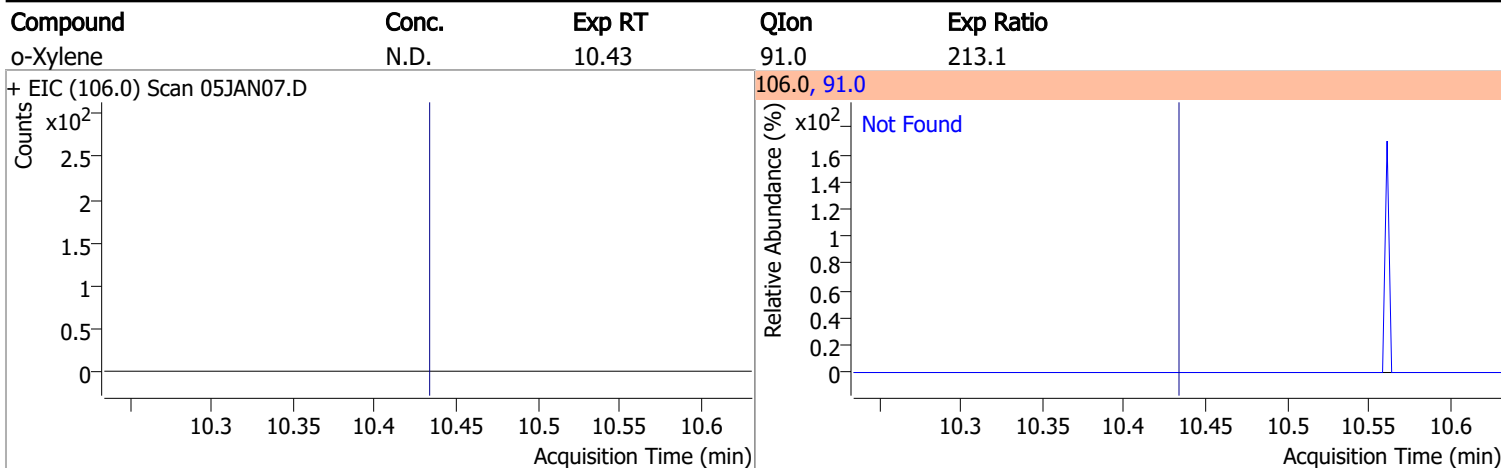









| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 282.2742 | 10.95 | 0.00 | 199881 | 174.0 | 94.9 | 61.7 | 121.7 |
| | | | | | 176.0 | 91.6 | 60.6 | 120.6 |



Quantitation Results Report (QT Reviewed)

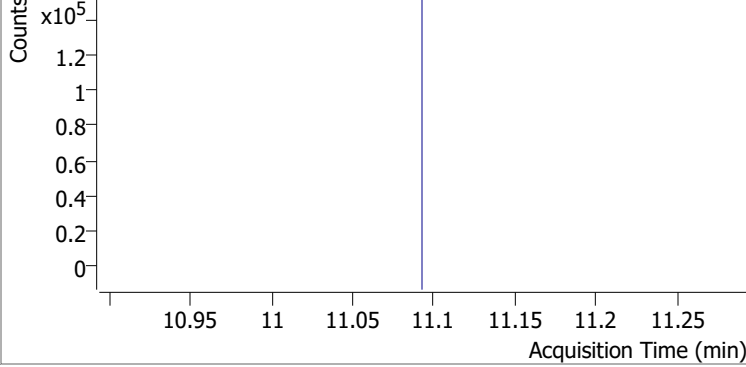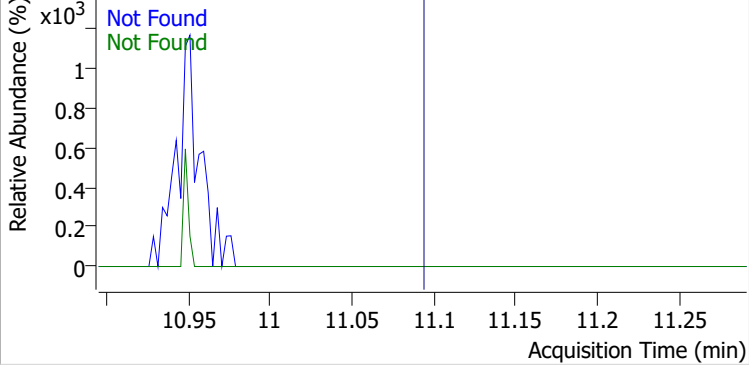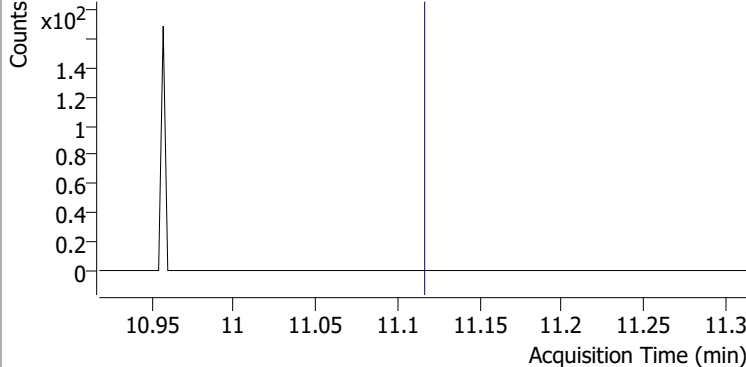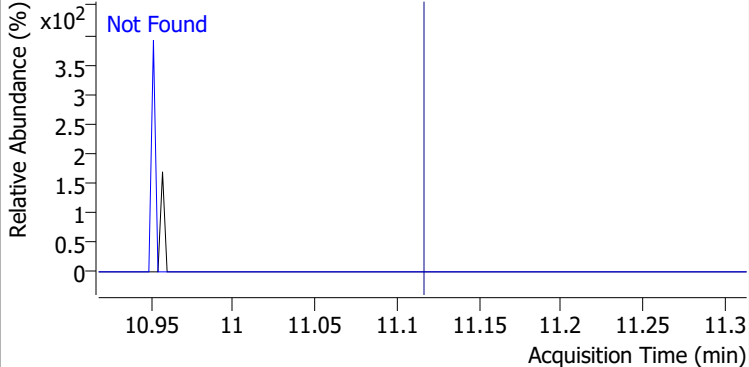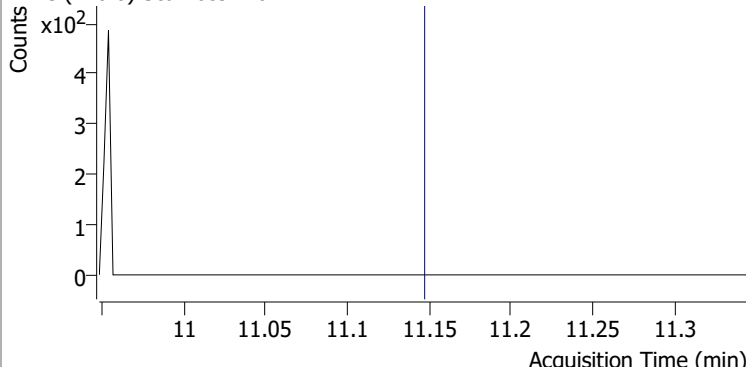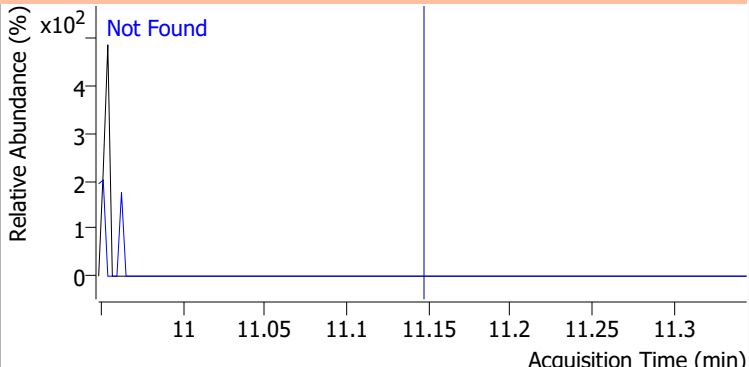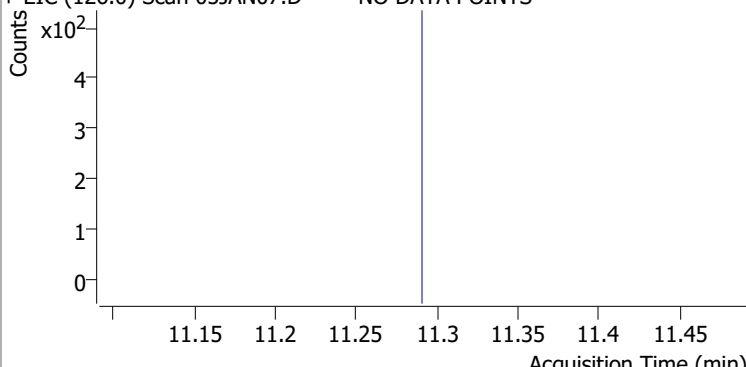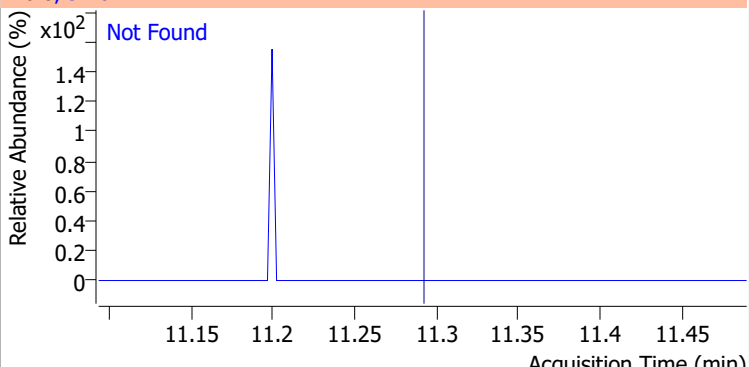
| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--|-------|--------|--|-----------|-------|-----------|
| Bromobenzene | N.D. | 11.09 | 77.0 | 145.7 | 158.0 | 96.5 |
| + EIC (156.0) Scan 05JAN07.D ***NO DATA POINTS*** | | | 156.0, 77.0, 158.0 | | | |
|  | | |  | | | |
| 1,1,2,2-Tetrachloroethane | N.D. | 11.12 | 85.0 | 66.2 | | |
| + EIC (83.0) Scan 05JAN07.D | | | 83.0, 85.0 | | | |
|  | | |  | | | |
| 1,2,3-Trichloropropane | N.D. | 11.15 | 112.0 | 63.5 | | |
| + EIC (110.0) Scan 05JAN07.D | | | 110.0, 112.0 | | | |
|  | | |  | | | |
| 2-Chlorotoluene | N.D. | 11.29 | 91.0 | 282.3 | | |
| + EIC (126.0) Scan 05JAN07.D ***NO DATA POINTS*** | | | 126.0, 91.0 | | | |
|  | | |  | | | |

Quantitation Results Report (QT Reviewed)
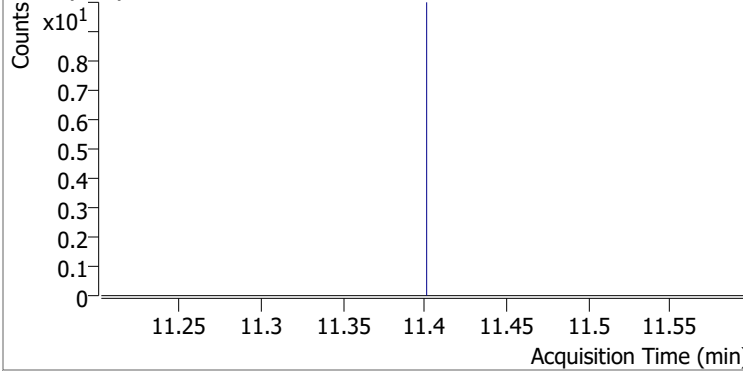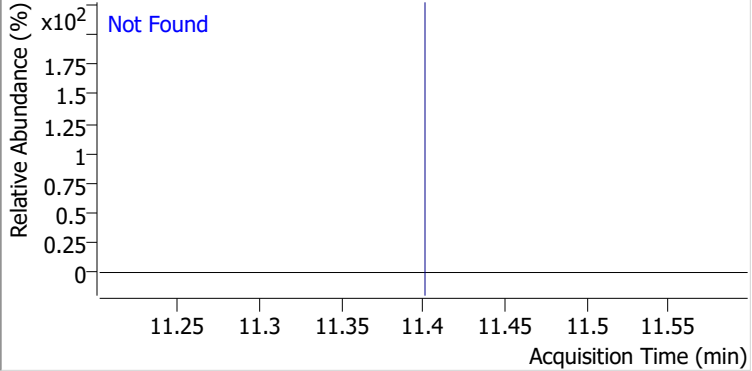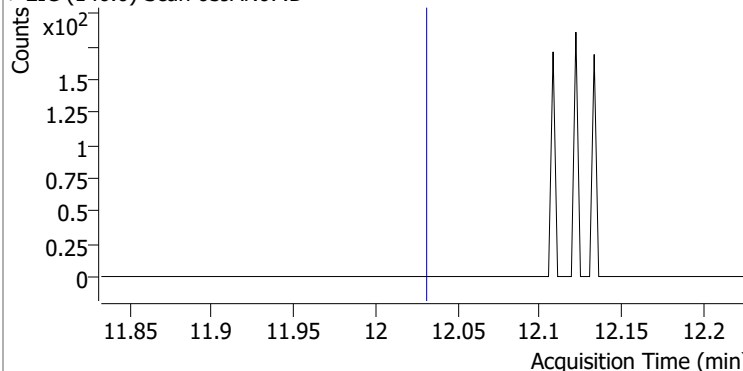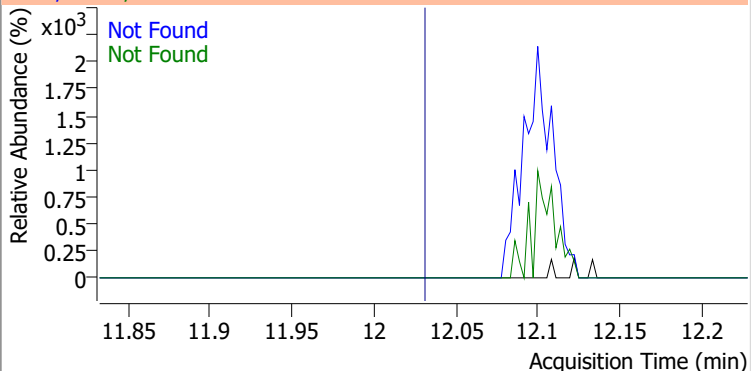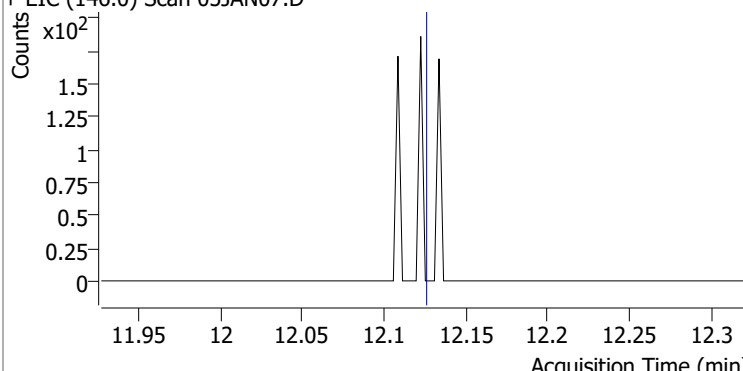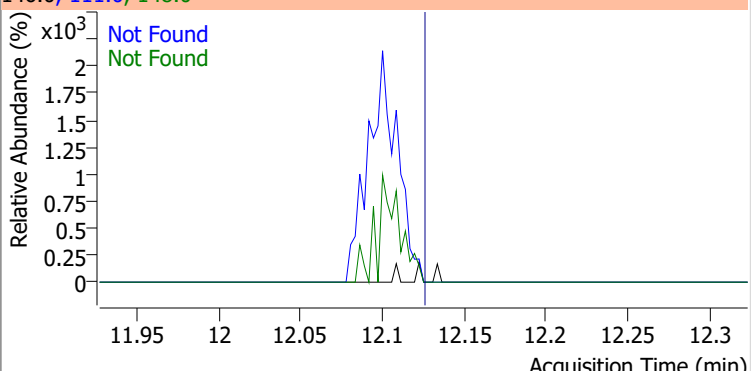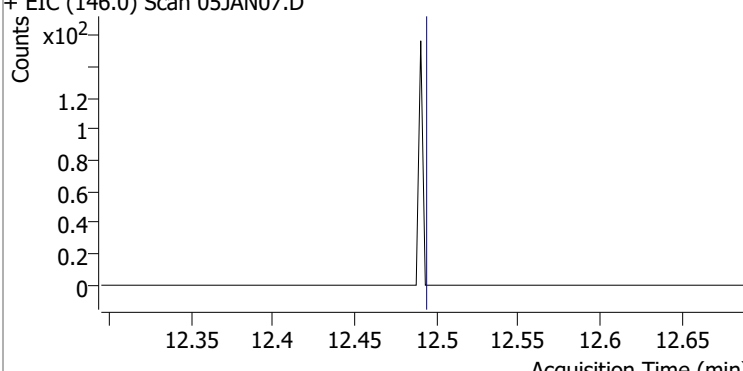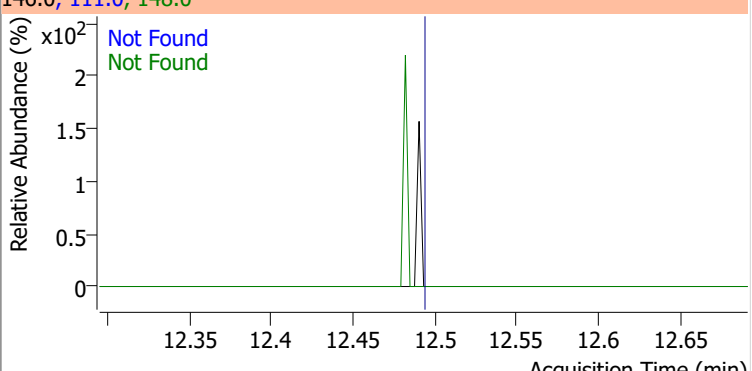
| Compound | Conc. | Exp RT | QIon | Exp Ratio | | |
|--|-------|--------|--|-----------|------|-----------|
| 4-Chlorotoluene | N.D. | 11.40 | 126.0 | 31.7 | | |
| + EIC (91.0) Scan 05JAN07.D | | | 91.0, 126.0 | | | |
|  | | |  | | | |
| 1,3-Dichlorobenzene | N.D. | 12.03 | 148.0 | 63.6 | QIon | Exp Ratio |
| + EIC (146.0) Scan 05JAN07.D | | | 146.0, 111.0, 148.0 | | | |
|  | | |  | | | |
| 1,4-Dichlorobenzene | N.D. | 12.13 | 148.0 | 63.1 | QIon | Exp Ratio |
| + EIC (146.0) Scan 05JAN07.D | | | 146.0, 111.0, 148.0 | | | |
|  | | |  | | | |
| 1,2-Dichlorobenzene | N.D. | 12.49 | 148.0 | 63.9 | QIon | Exp Ratio |
| + EIC (146.0) Scan 05JAN07.D | | | 146.0, 111.0, 148.0 | | | |
|  | | |  | | | |

Quantitation Results Report (QT Reviewed)

| | | | |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File | 05JAN08.D | Operator | MSC |
| Acq. Method | 5975CACQF.M | Acq. Date-Time | 1/5/2022 1:16:30 PM |
| Sample Name | B22010096-002A | Instrument | VOA5975C |
| Vial | 8 | Multiplier | 1.00 |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m | Comment | |
| Tune File | BFB_Atune3.u | Tune Date | 10/11/2021 4:02:00 PM |
| Batch Name | VG010522_8260B.batch.bin | Last Calib Update | 2/28/2022 2:48:47 PM |
| Ref Library | \\MASSHUNTER\Org\Library\NIST129K.I | | |







| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|--------------------|-------|----------|
| Internal Standards | | | | | | |
| M Fluorobenzene | 6.618 | 96.0 | 737623 | 250.0000 | ng | -0.006 |
| M Chlorobenzene-d5 | 9.774 | 82.0 | 286149 | 250.0000 | ng | 0.003 |
| M 1,4-Dichlorobenzene-d4 | 12.100 | 152.0 | 220564 | 250.0000 | ng | 0.000 |
| System Monitoring Compounds | | | | | | |
| S Dibromofluoromethane | 5.848 | 113.0 | 194476 | 279.8555 | ng | 0.003 |
| Spiked Amount: 250.000 | Range: 80.0 - 119.0% | | | Recovery = 111.94% | | |
| S 1,2-Dichloroethane-d4 | 6.235 | 67.0 | 87038 | 289.9783 | ng | 0.003 |
| Spiked Amount: 250.000 | Range: 81.0 - 118.0% | | | Recovery = 115.99% | | |
| S Toluene-d8 | 8.321 | 98.0 | 729963 | 264.7213 | ng | 0.003 |
| Spiked Amount: 250.000 | Range: 89.0 - 112.0% | | | Recovery = 105.89% | | |
| S p-Bromofluorobenzene | 10.951 | 95.0 | 217958 | 269.7370 | ng | -0.003 |
| Spiked Amount: 250.000 | Range: 85.0 - 114.0% | | | Recovery = 107.89% | | |
| Target Compounds | | | | | | |
| T Dichlorodifluoromethane | 0.000 | | 0 | N.D. | | |
| T Chloromethane | 1.406 | 50.0 | 4181 | 3.5637 | ng | 95 |
| T Vinyl chloride | 0.000 | | 0 | N.D. | | |
| T Bromomethane | 0.000 | | 0 | N.D. | | |
| T Chloroethane | 0.000 | | 0 | N.D. | | |
| T Trichlorofluoromethane | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methylene chloride | 3.324 | 49.0 | 1786 | 1.6309 | ng | m 89 |
| T trans-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methyl tert-butyl ether (MTBE) | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloroethane | 0.000 | | 0 | N.D. | | |
| T 2,2-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T cis-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methyl ethyl ketone | 0.000 | | 0 | N.D. | | |
| T Bromochloromethane | 0.000 | | 0 | N.D. | | |
| T Chloroform | 0.000 | | 0 | N.D. | | |

Quantitation Results Report (QT Reviewed)

| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|-----------------------------|-------|------|-------|--------|-------|----------|
| T 1,1,1-Trichloroethane | 0.000 | | 0 | N.D. | | |
| T Carbon tetrachloride | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloropropene | 0.000 | | 0 | N.D. | | |
| T Benzene | 0.000 | | 0 | N.D. | | |
| T 1,2-Dichloroethane | 0.000 | | 0 | N.D. | | |
| T Trichloroethene | 0.000 | | 0 | N.D. | | |
| T 1,2-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T Dibromomethane | 0.000 | | 0 | N.D. | | |
| T Bromodichloromethane | 0.000 | | 0 | N.D. | | |
| T cis-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | |
| T Toluene | 8.386 | 92.0 | 1683 | 0.9037 | ng m | 82 |
| T trans-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | |
| T 1,1,2-Trichloroethane | 0.000 | | 0 | N.D. | | |
| T Tetrachloroethene | 0.000 | | 0 | N.D. | | |
| T 1,3-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T Chlorodibromomethane | 0.000 | | 0 | N.D. | | |
| T 1,2-Dibromoethane | 0.000 | | 0 | N.D. | | |
| T Chlorobenzene | 0.000 | | 0 | N.D. | | |
| T 1,1,1,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | |
| T Ethylbenzene | 0.000 | | 0 | N.D. | | |
| T m+p-Xylenes | 0.000 | | 0 | N.D. | | |
| T o-Xylene | 0.000 | | 0 | N.D. | | |
| T Styrene | 0.000 | | 0 | N.D. | | |
| T Bromoform | 0.000 | | 0 | N.D. | | |
| T Bromobenzene | 0.000 | | 0 | N.D. | | |
| T 1,1,2,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | |
| T 1,2,3-Trichloropropane | 0.000 | | 0 | N.D. | | |
| T 2-Chlorotoluene | 0.000 | | 0 | N.D. | | |
| T 4-Chlorotoluene | 0.000 | | 0 | N.D. | | |
| T 1,3-Dichlorobenzene | 0.000 | | 0 | N.D. | | |
| T 1,4-Dichlorobenzene | 0.000 | | 0 | N.D. | | |
| T 1,2-Dichlorobenzene | 0.000 | | 0 | N.D. | | |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)

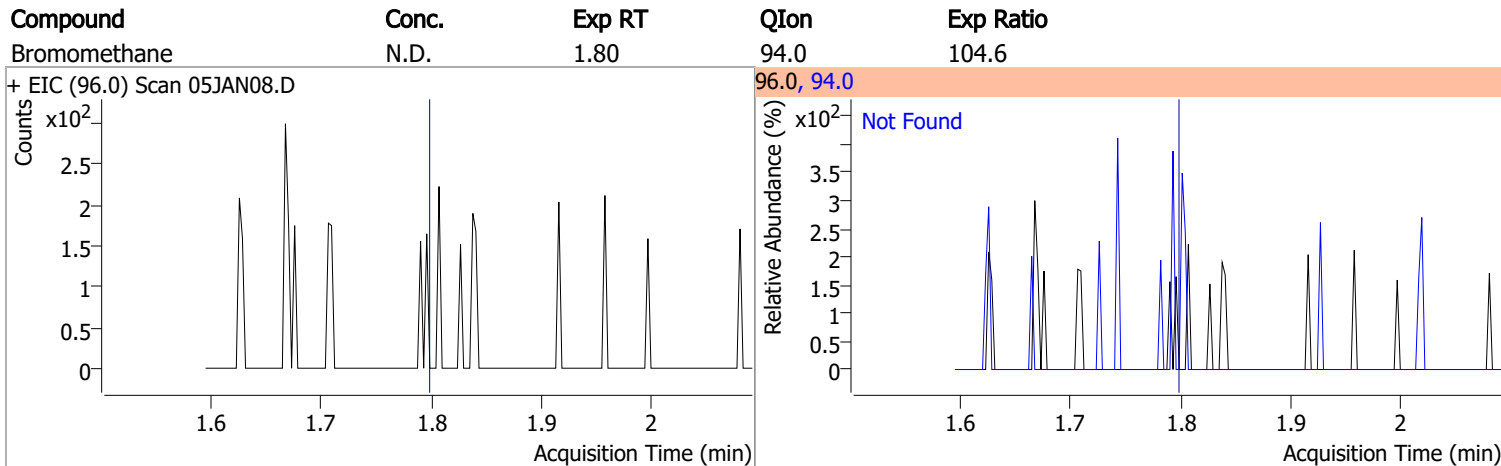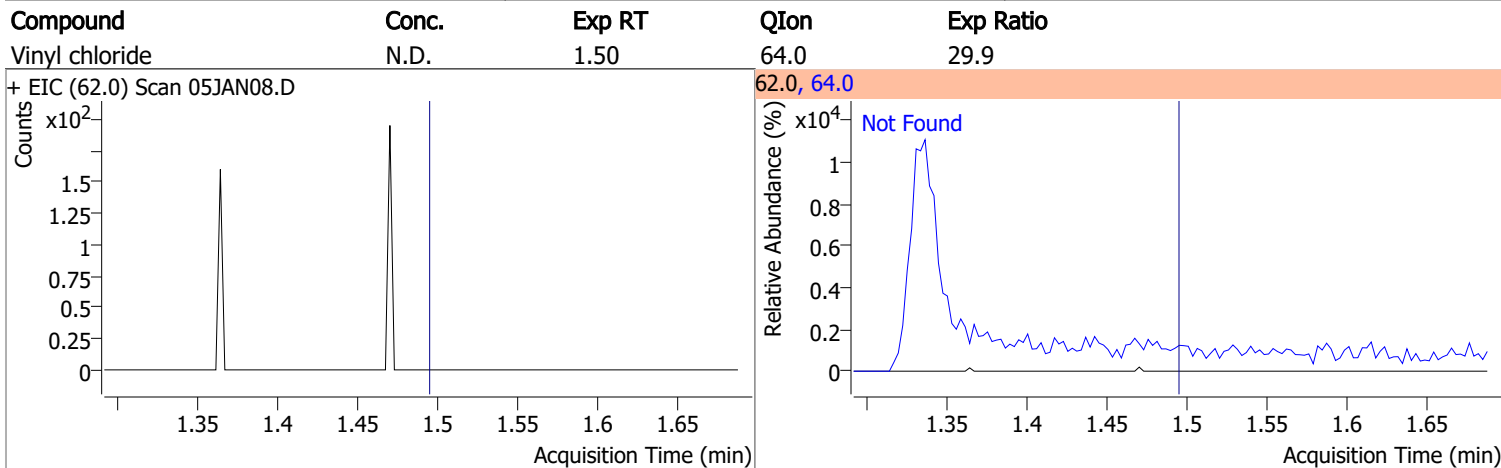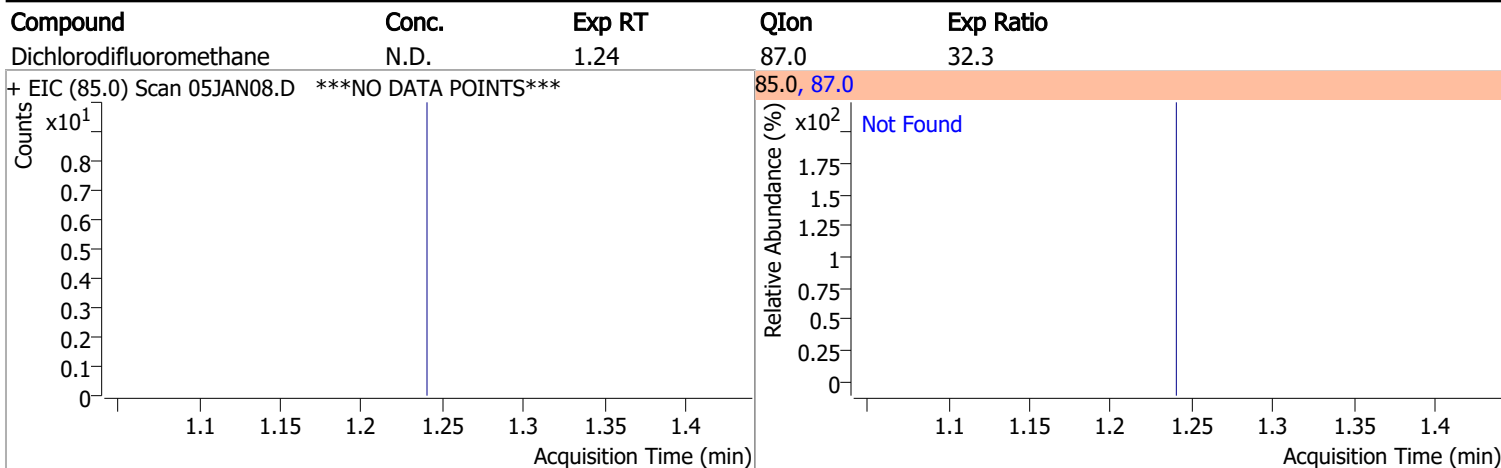


Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------|-------|--------|------|-----------|
| Chloroethane | N.D. | 1.89 | 66.0 | 30.1 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|------------------------|-------|--------|-------|-----------|
| Trichlorofluoromethane | N.D. | 2.14 | 103.0 | 64.2 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethene | N.D. | 2.70 | 61.0 | 180.3 | 63.0 | 56.7 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|--------|------|----------|----------|------|--------|-------|-------|
| Methylene chloride | 1.6309 | 3.32 | -0.01 | 1786 (m) | 84.0 | 59.9 | 36.9 | 96.9 |
| | | | | | 86.0 | 34.5 | 14.3 | 74.3 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,2-Dichloroethene | N.D. | 3.72 | 61.0 | 153.9 | 98.0 | 65.7 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------------------|-------|--------|------|-----------|
| Methyl tert-butyl ether (MTBE) | N.D. | 3.75 | 57.0 | 24.6 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethane | N.D. | 4.38 | 65.0 | 32.1 | 83.0 | 13.7 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|------|-----------|
| 2,2-Dichloropropane | N.D. | 5.20 | 41.0 | 66.5 | 97.0 | 23.2 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|------------------------|-------|--------|------|-----------|------|-----------|
| cis-1,2-Dichloroethene | N.D. | 5.22 | 61.0 | 167.2 | 98.0 | 67.3 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| Methyl ethyl ketone | N.D. | 5.28 | 72.0 | 21.3 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|
| Bromochloromethane | N.D. | 5.52 | 49.0 | 182.9 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|------------|-------|--------|------|-----------|
| Chloroform | N.D. | 5.65 | 85.0 | 66.0 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------------|-------|--------|------|-----------|------|-----------|
| 1,1,1-Trichloroethane | N.D. | 5.83 | 99.0 | 64.7 | 61.0 | 48.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Dibromofluoromethane | 279.8555 | 5.85 | 0.00 | 194476 | 191.5 | 22.3 | 0.0 | 53.1 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|----------------------|-------|--------|-------|-----------|-------|-----------|
| Carbon tetrachloride | N.D. | 6.02 | 119.0 | 97.2 | 121.0 | 30.1 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|-------|-----------|------|-----------|
| 1,1-Dichloropropene | N.D. | 6.04 | 110.0 | 35.9 | 77.0 | 30.1 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 289.9783 | 6.24 | 0.00 | 87038 | 65.0 | 197.5 | 166.5 | 226.5 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------|-------|--------|------|-----------|
| Benzene | N.D. | 6.28 | 77.0 | 23.5 |







| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,2-Dichloroethane | N.D. | 6.32 | 64.0 | 29.9 | 98.0 | 7.6 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------|-------|--------|-------|-----------|------|-----------|
| Trichloroethene | N.D. | 7.03 | 130.0 | 101.5 | 97.0 | 64.1 |




Quantitation Results Report (QT Reviewed)

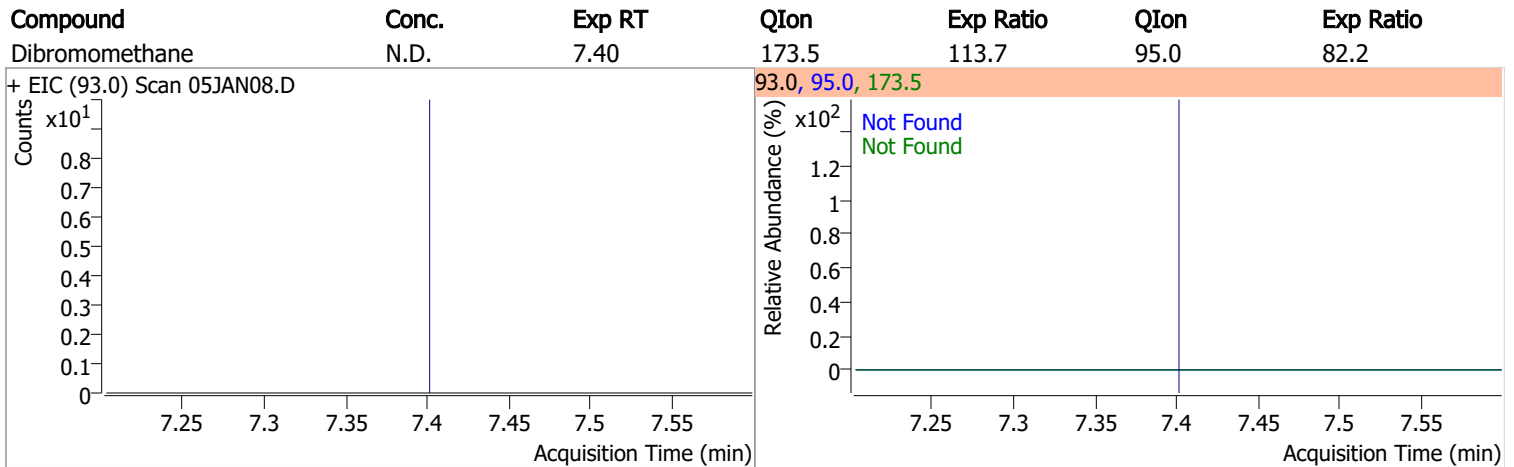


Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 264.7213 | 8.32 | 0.00 | 729963 | 100.0 | 64.4 | 34.4 | 94.4 |
| | | | | | 99.0 | 9.3 | 0.0 | 39.6 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|--------|------|----------|----------|------|--------|-------|-------|
| Toluene | 0.9037 | 8.39 | 0.00 | 1683 (m) | 91.0 | 150.9 | 145.8 | 205.8 |











| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,3-Dichloropropene | N.D. | 8.64 | 39.0 | 53.4 | 77.0 | 32.4 |











| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------------|-------|--------|------|-----------|------|-----------|
| 1,1,2-Trichloroethane | N.D. | 8.82 | 97.0 | 114.6 | 85.0 | 67.6 |






Quantitation Results Report (QT Reviewed)
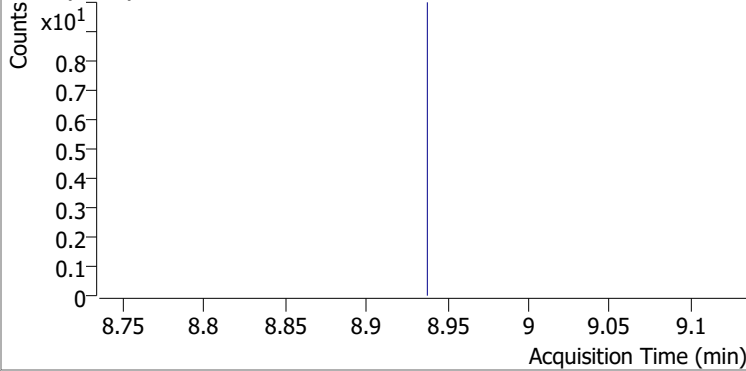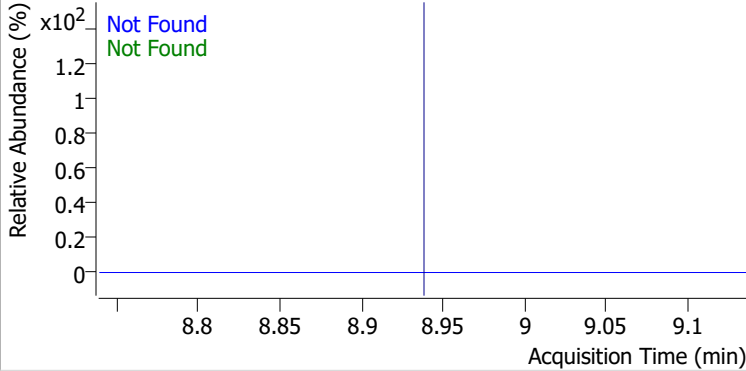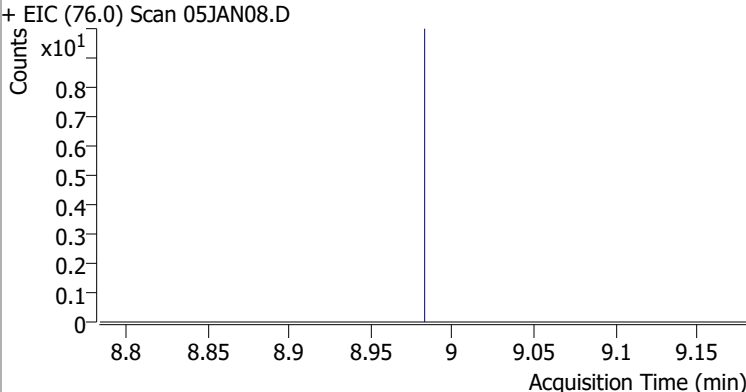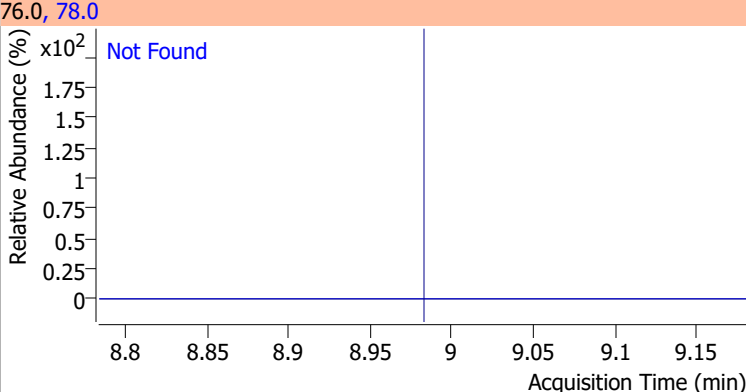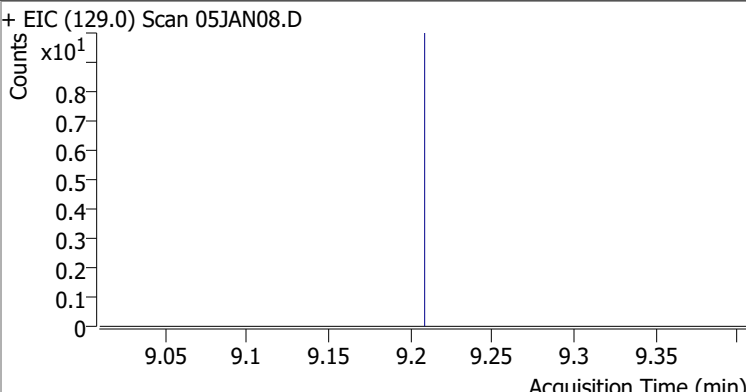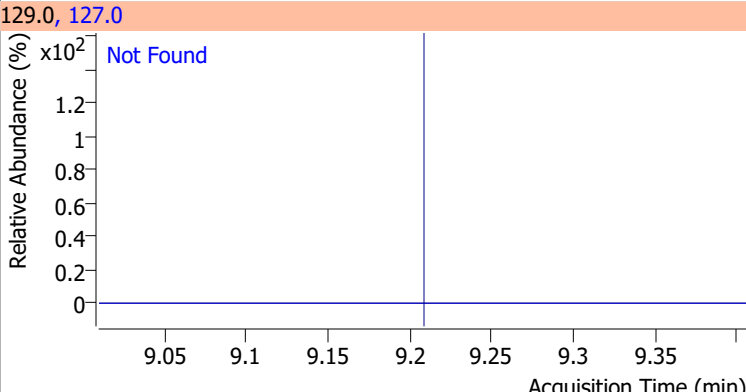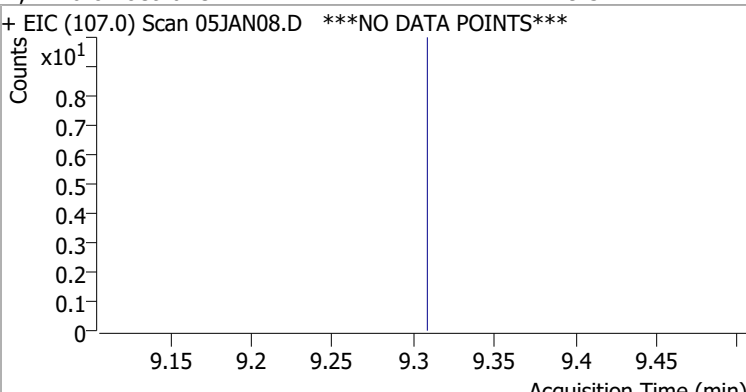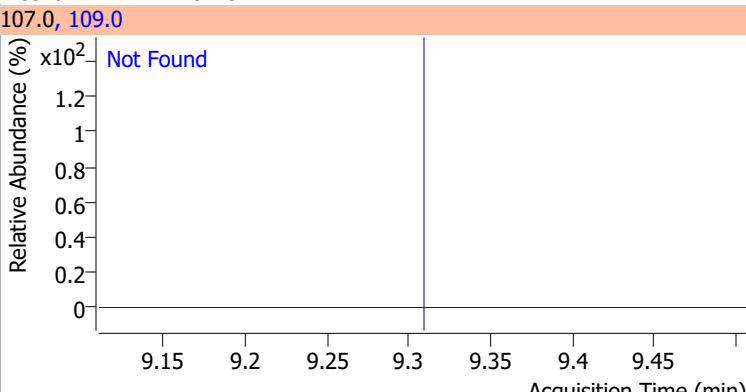
| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--|-------|--------|--|-----------|-------|-----------|
| Tetrachloroethene | N.D. | 8.94 | 165.8 | 128.6 | 129.0 | 91.5 |
| + EIC (163.8) Scan 05JAN08.D ***NO DATA POINTS*** | | | 163.8, 129.0, 165.8 | | | |
|  | | |  | | | |
| 1,3-Dichloropropane | N.D. | 8.98 | 78.0 | 32.9 | | |
| + EIC (76.0) Scan 05JAN08.D | | | 76.0, 78.0 | | | |
|  | | |  | | | |
| Chlorodibromomethane | N.D. | 9.21 | 127.0 | 78.0 | | |
| + EIC (129.0) Scan 05JAN08.D | | | 129.0, 127.0 | | | |
|  | | |  | | | |
| 1,2-Dibromoethane | N.D. | 9.31 | 109.0 | 94.5 | | |
| + EIC (107.0) Scan 05JAN08.D ***NO DATA POINTS*** | | | 107.0, 109.0 | | | |
|  | | |  | | | |


Quantitation Results Report (QT Reviewed)
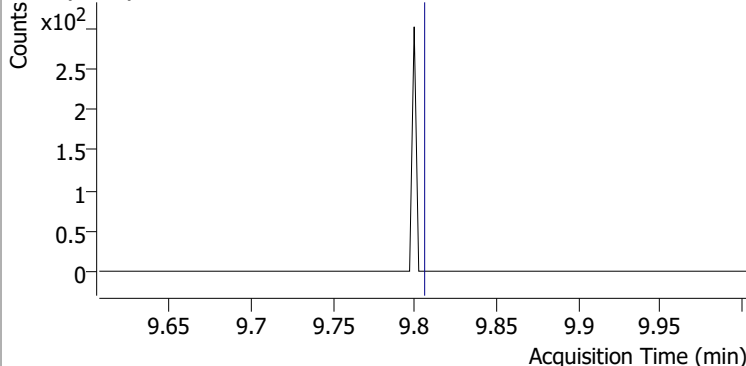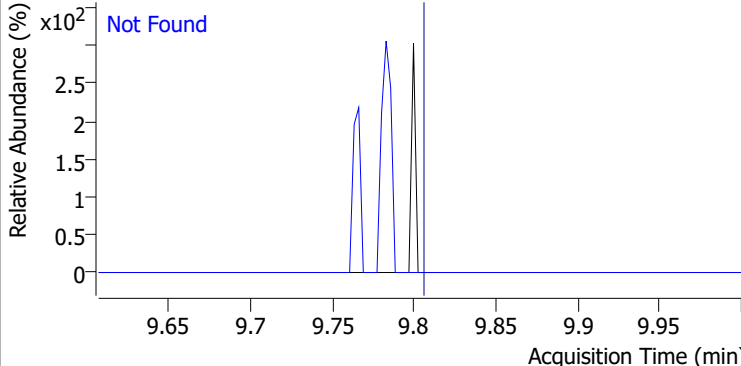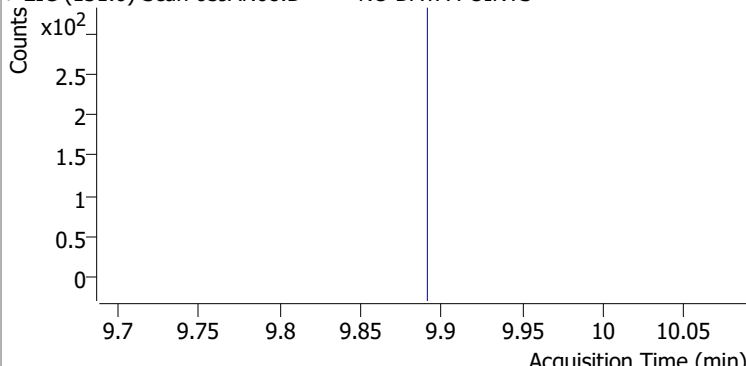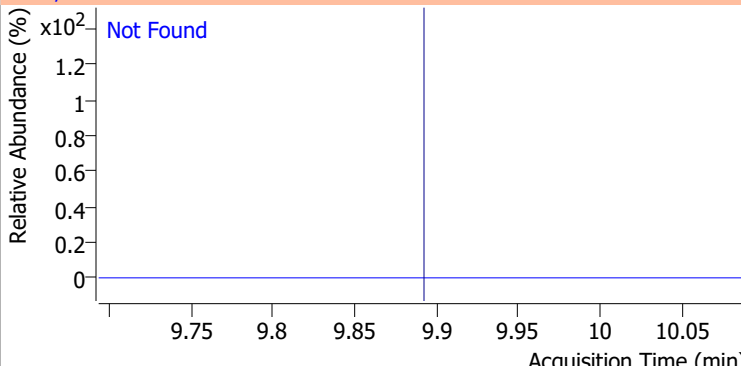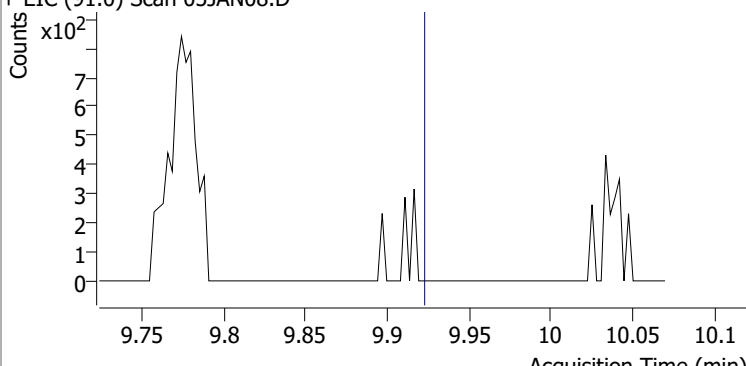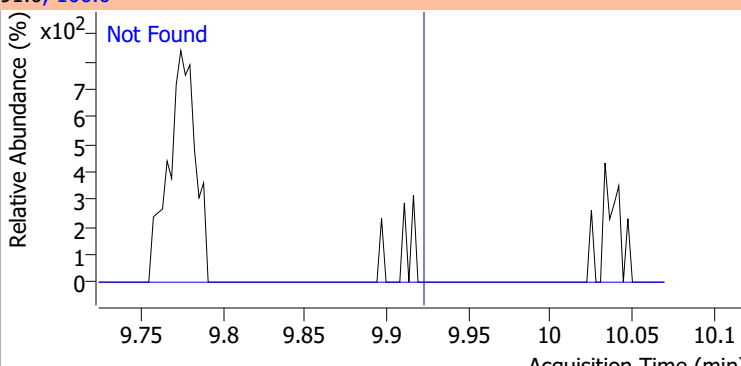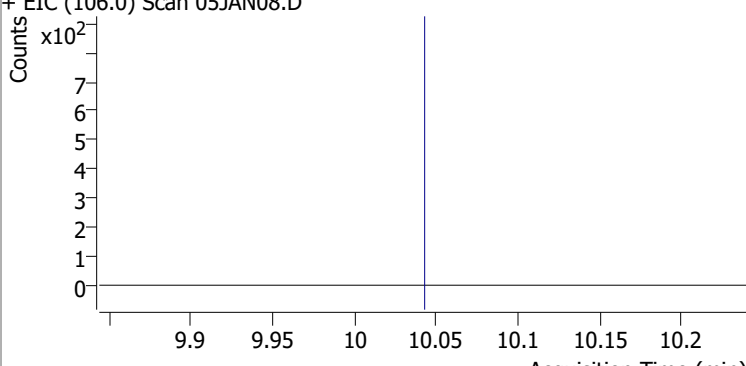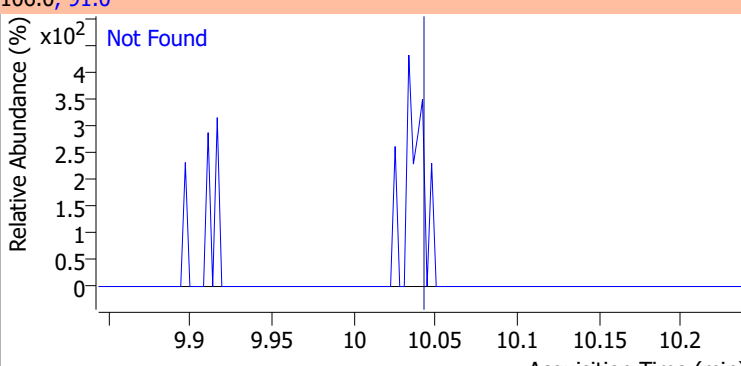
| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--|-------|--------|--|-----------|
| Chlorobenzene | N.D. | 9.80 | 114.0 | 32.1 |
| + EIC (112.0) Scan 05JAN08.D | | | 112.0, 114.0 | |
|  | | |  | |
| 1,1,1,2-Tetrachloroethane | N.D. | 9.89 | 133.0 | 98.6 |
| + EIC (131.0) Scan 05JAN08.D ***NO DATA POINTS*** | | | 131.0, 133.0 | |
|  | | |  | |
| Ethylbenzene | N.D. | 9.92 | 106.0 | 31.1 |
| + EIC (91.0) Scan 05JAN08.D | | | 91.0, 106.0 | |
|  | | |  | |
| m+p-Xylenes | N.D. | 10.04 | 91.0 | 201.4 |
| + EIC (106.0) Scan 05JAN08.D | | | 106.0, 91.0 | |
|  | | |  | |

Quantitation Results Report (QT Reviewed)

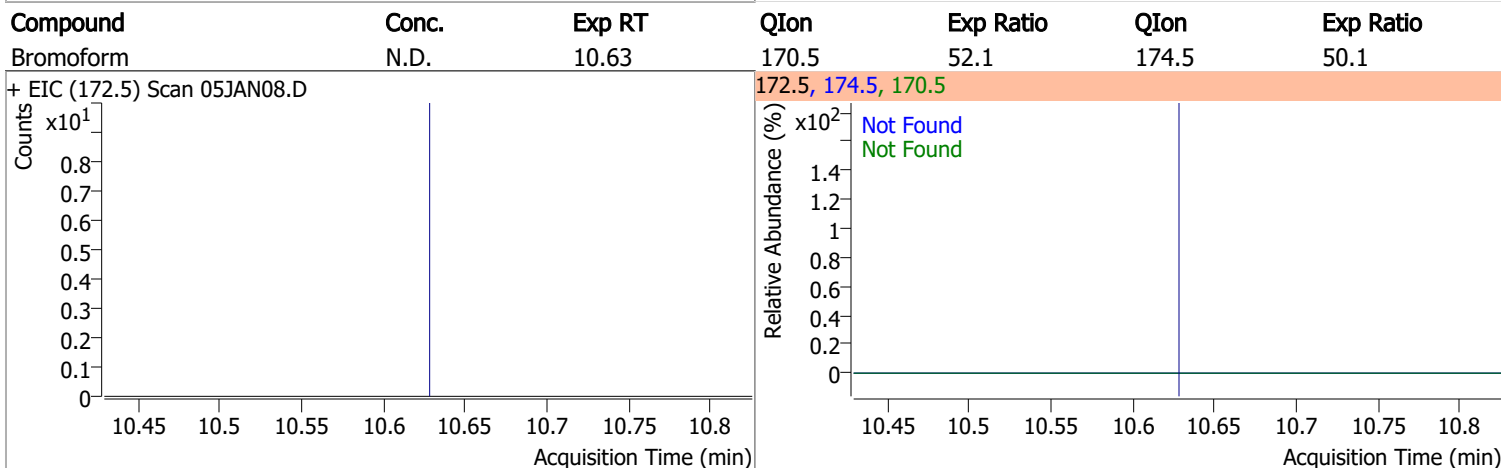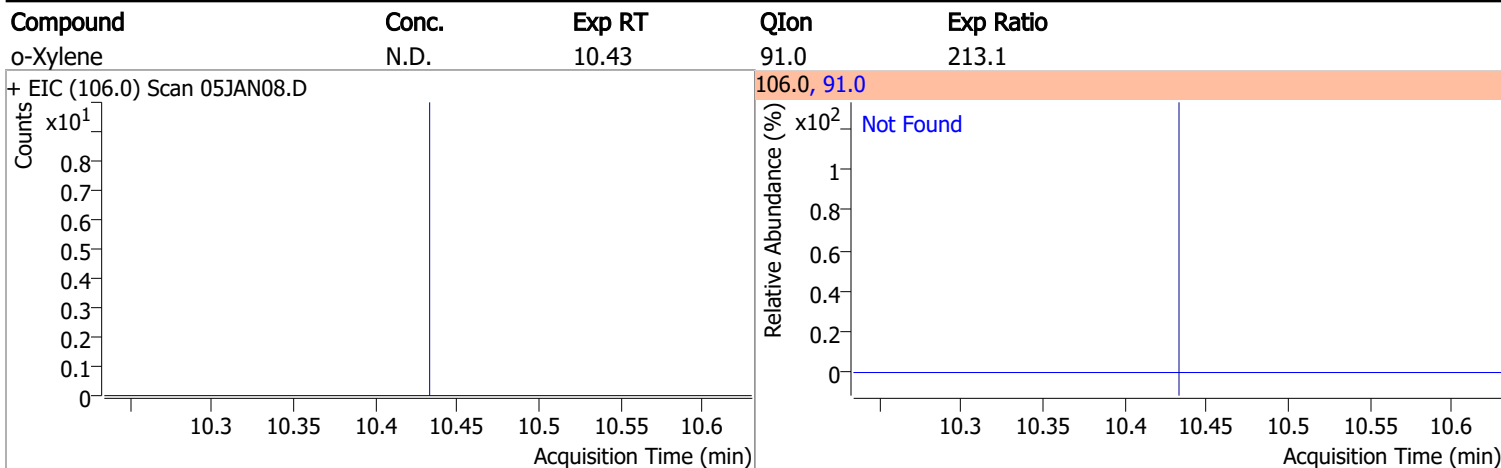


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 269.7370 | 10.95 | 0.00 | 217958 | 174.0 | 93.1 | 61.7 | 121.7 |
| | | | | | 176.0 | 90.2 | 60.6 | 120.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------|-------|--------|------|-----------|-------|-----------|
| Bromobenzene | N.D. | 11.09 | 77.0 | 145.7 | 158.0 | 96.5 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------------|-------|--------|------|-----------|
| 1,1,2,2-Tetrachloroethane | N.D. | 11.12 | 85.0 | 66.2 |











| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|------------------------|-------|--------|-------|-----------|
| 1,2,3-Trichloropropane | N.D. | 11.15 | 112.0 | 63.5 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|-----------------|-------|--------|------|-----------|
| 2-Chlorotoluene | N.D. | 11.29 | 91.0 | 282.3 |




Quantitation Results Report (QT Reviewed)
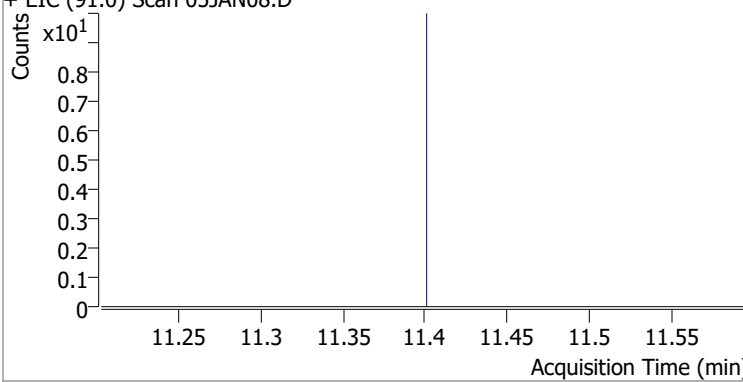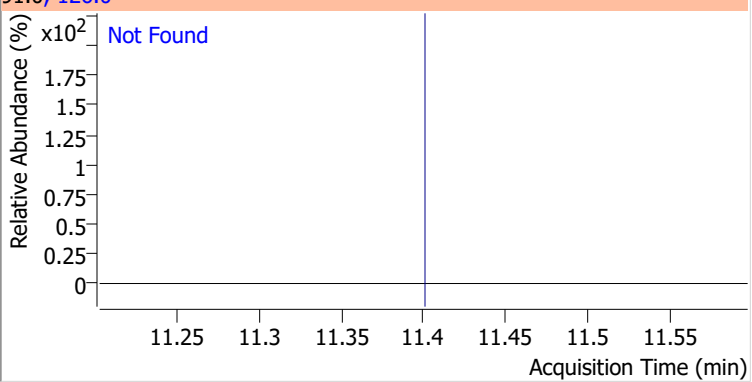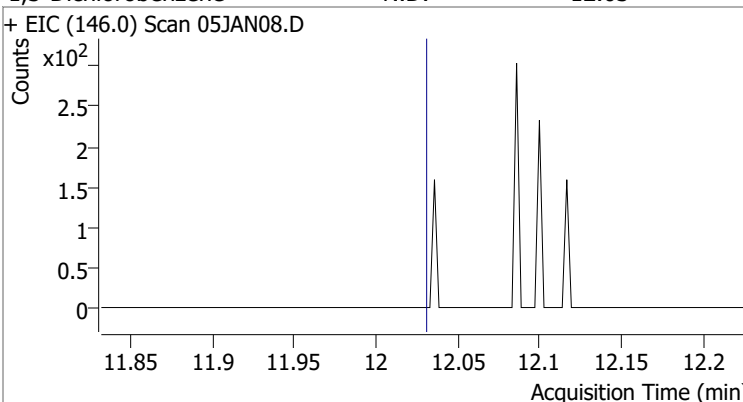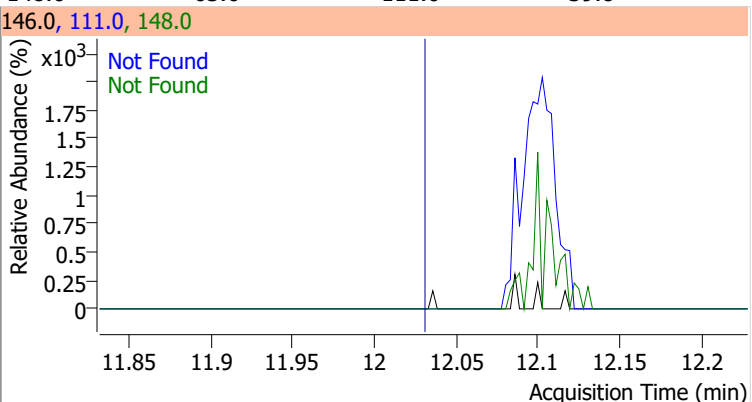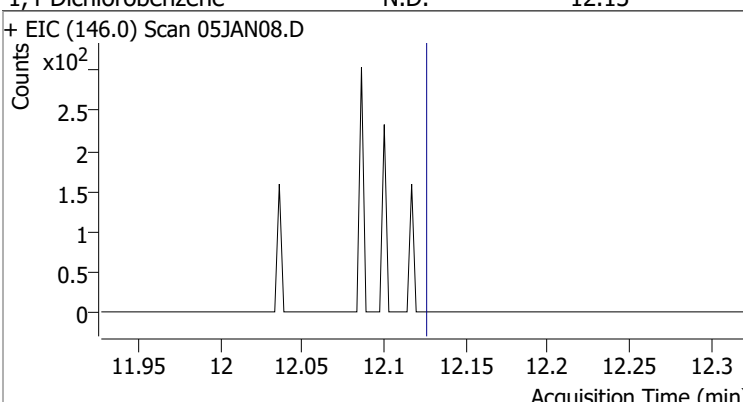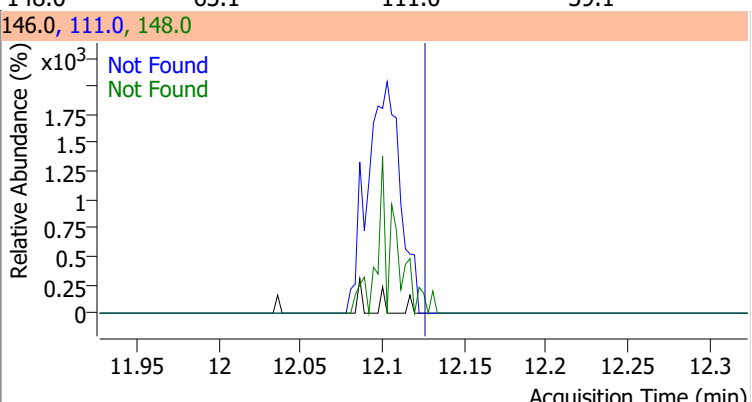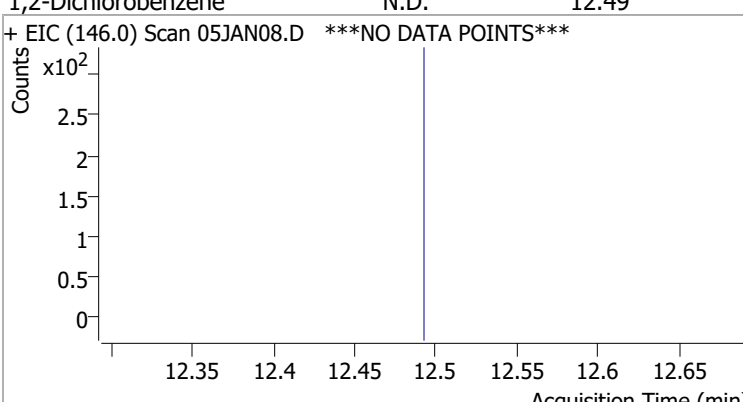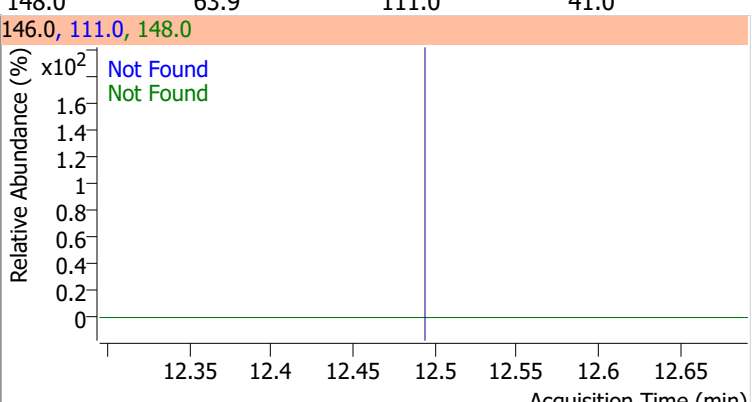
| Compound | Conc. | Exp RT | QIon | Exp Ratio | | |
|--|-------|--------|--|-----------|------|-----------|
| 4-Chlorotoluene | N.D. | 11.40 | 126.0 | 31.7 | | |
| + EIC (91.0) Scan 05JAN08.D | | | 91.0, 126.0 | | | |
|  | | |  | | | |
| 1,3-Dichlorobenzene | N.D. | 12.03 | 148.0 | 63.6 | QIon | Exp Ratio |
| + EIC (146.0) Scan 05JAN08.D | | | 146.0, 111.0, 148.0 | | | |
|  | | |  | | | |
| 1,4-Dichlorobenzene | N.D. | 12.13 | 148.0 | 63.1 | QIon | Exp Ratio |
| + EIC (146.0) Scan 05JAN08.D | | | 146.0, 111.0, 148.0 | | | |
|  | | |  | | | |
| 1,2-Dichlorobenzene | N.D. | 12.49 | 148.0 | 63.9 | QIon | Exp Ratio |
| + EIC (146.0) Scan 05JAN08.D ***NO DATA POINTS*** | | | 146.0, 111.0, 148.0 | | | |
|  | | |  | | | |

Quantitation Results Report (QT Reviewed)

| | | | |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File | 05JAN09.D | Operator | MSC |
| Acq. Method | 5975CACQF.M | Acq. Date-Time | 1/5/2022 1:43:48 PM |
| Sample Name | B22010120-002A | Instrument | VOA5975C |
| Vial | 9 | Multiplier | 1.00 |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m | Comment | |
| Tune File | BFB_Atune3.u | Tune Date | 10/11/2021 4:02:00 PM |
| Batch Name | VG010522_8260B.batch.bin | Last Calib Update | 2/28/2022 2:48:47 PM |
| Ref Library | \\MASSHUNTER\Org\Library\NIST129K.I | | |







| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|----------------------|-------|----------|
| Internal Standards | | | | | | |
| M Fluorobenzene | 6.623 | 96.0 | 725823 | 250.0000 | ng | 0.000 |
| M Chlorobenzene-d5 | 9.774 | 82.0 | 284050 | 250.0000 | ng | 0.003 |
| M 1,4-Dichlorobenzene-d4 | 12.100 | 152.0 | 218466 | 250.0000 | ng | 0.000 |
| System Monitoring Compounds | | | | | | |
| S Dibromofluoromethane | 5.851 | 113.0 | 193743 | 283.3333 | ng | 0.005 |
| Spiked Amount: 250.000 | Range: 80.0 - 119.0% | | | Recovery = 113.33% | | |
| S 1,2-Dichloroethane-d4 | 6.230 | 67.0 | 87408 | 295.9454 | ng | -0.003 |
| Spiked Amount: 250.000 | Range: 81.0 - 118.0% | | | Recovery = 118.38% * | | |
| S Toluene-d8 | 8.321 | 98.0 | 741100 | 270.7461 | ng | 0.003 |
| Spiked Amount: 250.000 | Range: 89.0 - 112.0% | | | Recovery = 108.30% | | |
| S p-Bromofluorobenzene | 10.951 | 95.0 | 214927 | 268.5403 | ng | -0.003 |
| Spiked Amount: 250.000 | Range: 85.0 - 114.0% | | | Recovery = 107.42% | | |
| Target Compounds | | | | | | |
| T Dichlorodifluoromethane | 0.000 | | 0 | N.D. | | |
| T Chloromethane | 1.411 | 50.0 | 4032 | 3.4926 | ng | 85 |
| T Vinyl chloride | 0.000 | | 0 | N.D. | | |
| T Bromomethane | 0.000 | | 0 | N.D. | | |
| T Chloroethane | 0.000 | | 0 | N.D. | | |
| T Trichlorofluoromethane | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methylene chloride | 3.335 | 49.0 | 1869 | 1.7346 | ng | m 91 |
| T trans-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methyl tert-butyl ether (MTBE) | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloroethane | 0.000 | | 0 | N.D. | | |
| T 2,2-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T cis-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methyl ethyl ketone | 0.000 | | 0 | N.D. | | |
| T Bromochloromethane | 0.000 | | 0 | N.D. | | |
| T Chloroform | 0.000 | | 0 | N.D. | | |

Quantitation Results Report (QT Reviewed)

| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|-----------------------------|-------|------|-------|-------|-------|----------|
| T 1,1,1-Trichloroethane | 0.000 | | 0 | N.D. | | |
| T Carbon tetrachloride | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloropropene | 0.000 | | 0 | N.D. | | |
| T Benzene | 0.000 | | 0 | N.D. | | |
| T 1,2-Dichloroethane | 0.000 | | 0 | N.D. | | |
| T Trichloroethene | 0.000 | | 0 | N.D. | | |
| T 1,2-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T Dibromomethane | 0.000 | | 0 | N.D. | | |
| T Bromodichloromethane | 0.000 | | 0 | N.D. | | |
| T cis-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | |
| T Toluene | 8.391 | 92.0 | 0 | | ng md | 1 |
| T trans-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | |
| T 1,1,2-Trichloroethane | 0.000 | | 0 | N.D. | | |
| T Tetrachloroethene | 0.000 | | 0 | N.D. | | |
| T 1,3-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T Chlorodibromomethane | 0.000 | | 0 | N.D. | | |
| T 1,2-Dibromoethane | 0.000 | | 0 | N.D. | | |
| T Chlorobenzene | 0.000 | | 0 | N.D. | | |
| T 1,1,1,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | |
| T Ethylbenzene | 0.000 | | 0 | N.D. | | |
| T m+p-Xylenes | 0.000 | | 0 | N.D. | | |
| T o-Xylene | 0.000 | | 0 | N.D. | | |
| T Styrene | 0.000 | | 0 | N.D. | | |
| T Bromoform | 0.000 | | 0 | N.D. | | |
| T Bromobenzene | 0.000 | | 0 | N.D. | | |
| T 1,1,2,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | |
| T 1,2,3-Trichloropropane | 0.000 | | 0 | N.D. | | |
| T 2-Chlorotoluene | 0.000 | | 0 | N.D. | | |
| T 4-Chlorotoluene | 0.000 | | 0 | N.D. | | |
| T 1,3-Dichlorobenzene | 0.000 | | 0 | N.D. | | |
| T 1,4-Dichlorobenzene | 0.000 | | 0 | N.D. | | |
| T 1,2-Dichlorobenzene | 0.000 | | 0 | N.D. | | |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)

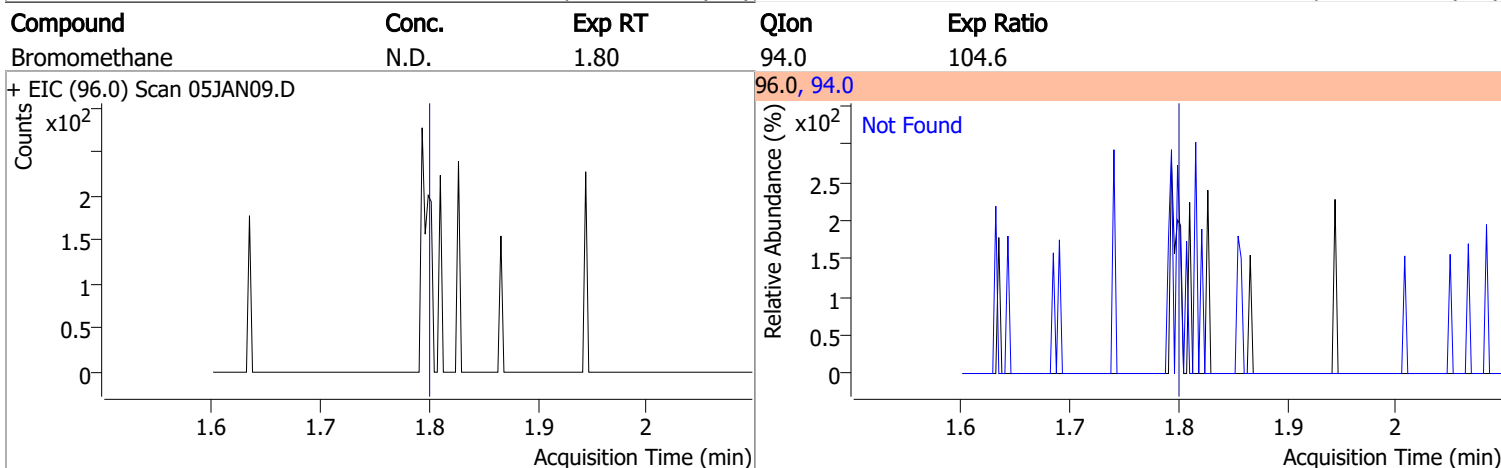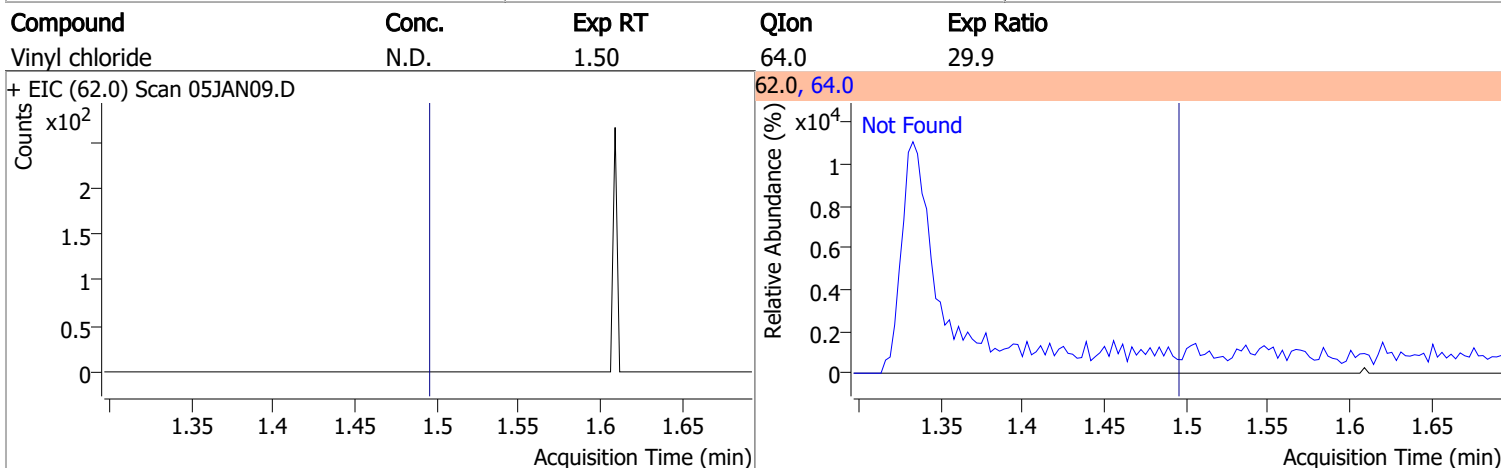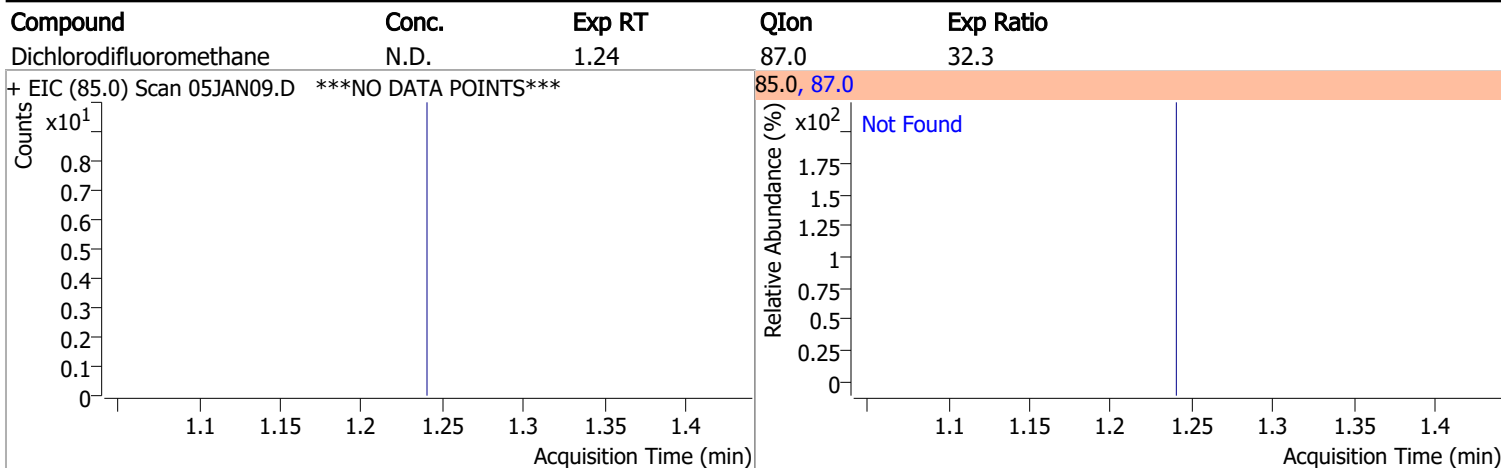


Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------|-------|--------|------|-----------|
| Chloroethane | N.D. | 1.89 | 66.0 | 30.1 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|------------------------|-------|--------|-------|-----------|
| Trichlorofluoromethane | N.D. | 2.14 | 103.0 | 64.2 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethene | N.D. | 2.70 | 61.0 | 180.3 | 63.0 | 56.7 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|--------|------|----------|----------|------|--------|-------|-------|
| Methylene chloride | 1.7346 | 3.34 | 0.00 | 1869 (m) | 84.0 | 59.2 | 36.9 | 96.9 |
| | | | | | 86.0 | 39.7 | 14.3 | 74.3 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,2-Dichloroethene | N.D. | 3.72 | 61.0 | 153.9 | 98.0 | 65.7 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------------------|-------|--------|------|-----------|
| Methyl tert-butyl ether (MTBE) | N.D. | 3.75 | 57.0 | 24.6 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethane | N.D. | 4.38 | 65.0 | 32.1 | 83.0 | 13.7 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|------|-----------|
| 2,2-Dichloropropane | N.D. | 5.20 | 41.0 | 66.5 | 97.0 | 23.2 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|------------------------|-------|--------|------|-----------|------|-----------|
| cis-1,2-Dichloroethene | N.D. | 5.22 | 61.0 | 167.2 | 98.0 | 67.3 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| Methyl ethyl ketone | N.D. | 5.28 | 72.0 | 21.3 |







| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|
| Bromochloromethane | N.D. | 5.52 | 49.0 | 182.9 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|------------|-------|--------|------|-----------|
| Chloroform | N.D. | 5.65 | 85.0 | 66.0 |




Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 295.9454 | 6.23 | 0.00 | 87408 | 65.0 | 197.9 | 166.5 | 226.5 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------|-------|--------|------|-----------|
| Benzene | N.D. | 6.28 | 77.0 | 23.5 |







| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,2-Dichloroethane | N.D. | 6.32 | 64.0 | 29.9 | 98.0 | 7.6 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------|-------|--------|-------|-----------|------|-----------|
| Trichloroethene | N.D. | 7.03 | 130.0 | 101.5 | 97.0 | 64.1 |




Quantitation Results Report (QT Reviewed)

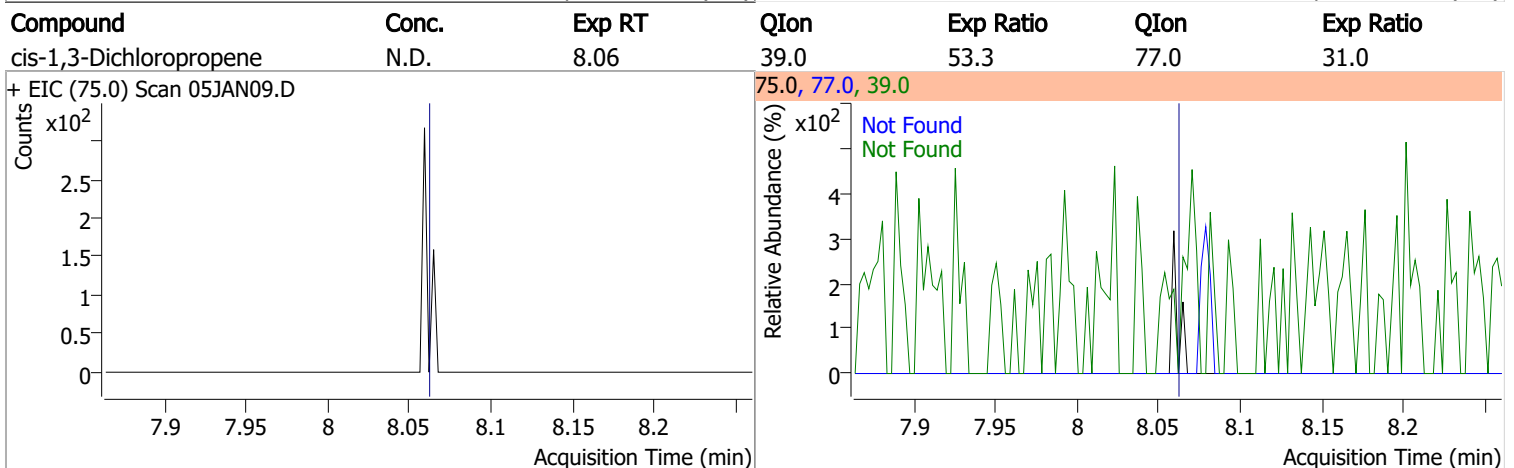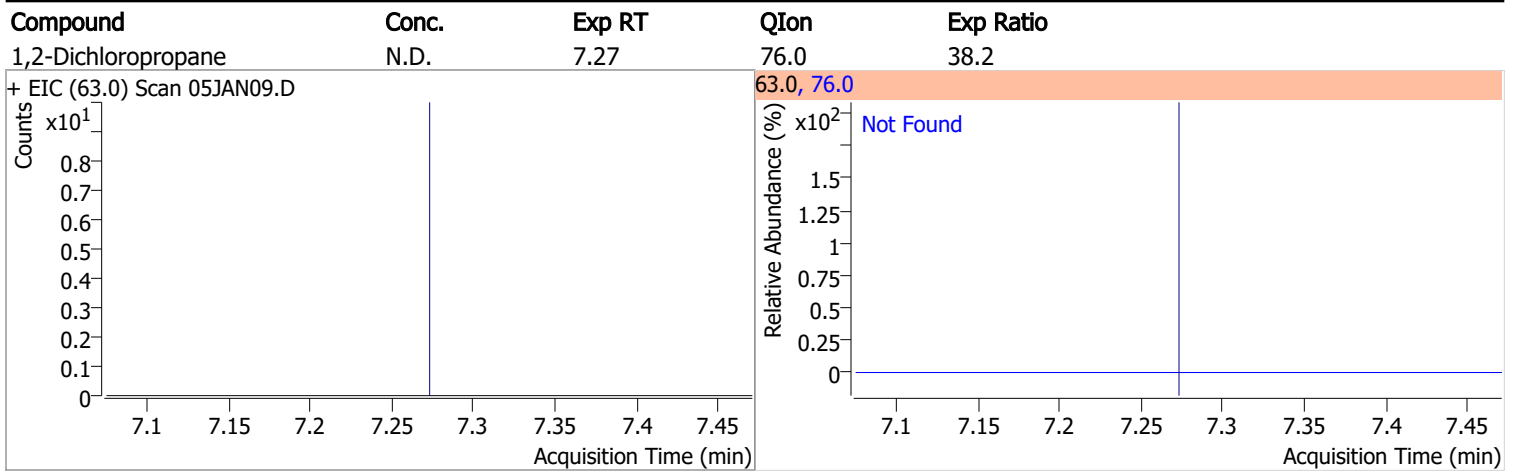


Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 270.7461 | 8.32 | 0.00 | 741100 | 100.0 | 63.0 | 34.4 | 94.4 |
| | | | | | 99.0 | 9.4 | 0.0 | 39.6 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|-------|----|----------|-------|------|--------|-------|-------|
| Toluene | 0 | 0 | 0 | 0 | 91.0 | 145.8 | 205.8 | |











| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,3-Dichloropropene | N.D. | 8.64 | 39.0 | 53.4 | 77.0 | 32.4 |











| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------------|-------|--------|------|-----------|------|-----------|
| 1,1,2-Trichloroethane | N.D. | 8.82 | 97.0 | 114.6 | 85.0 | 67.6 |






Quantitation Results Report (QT Reviewed)
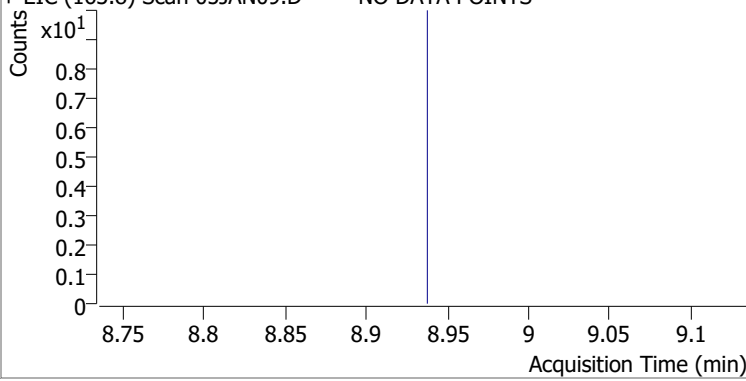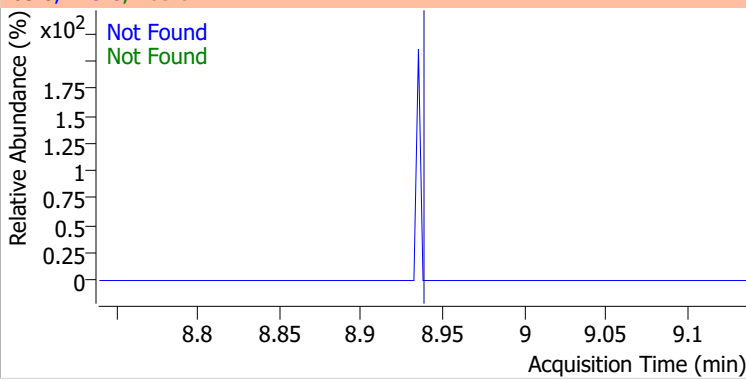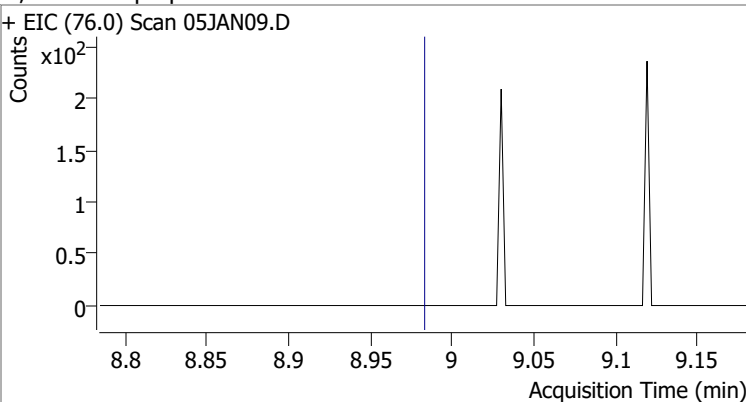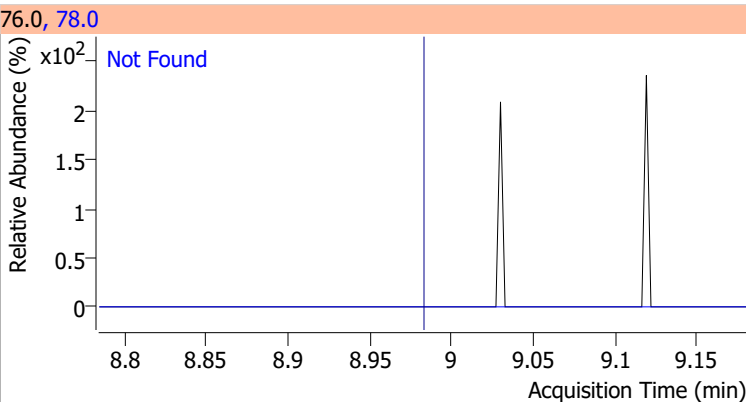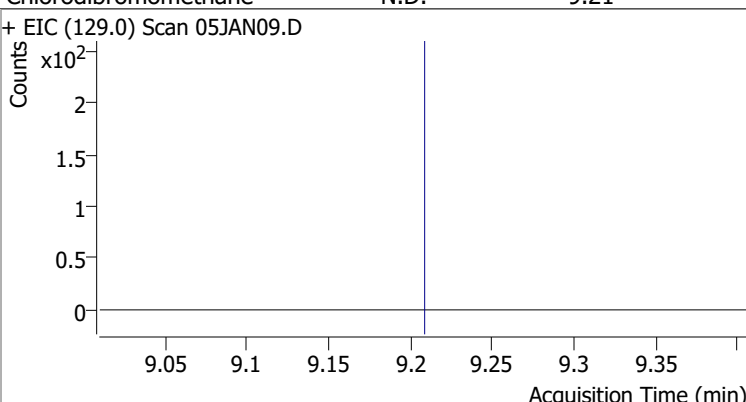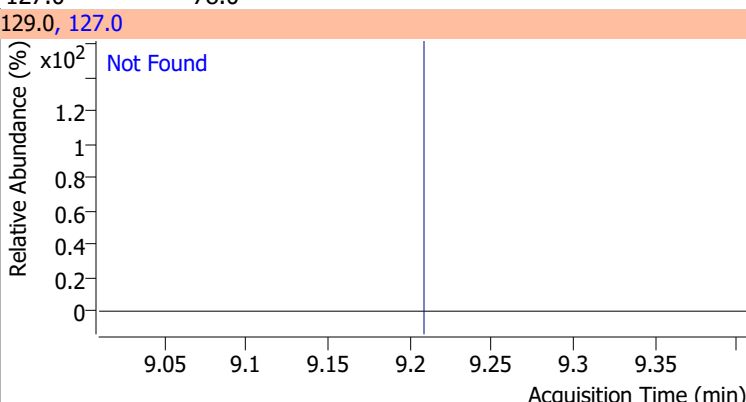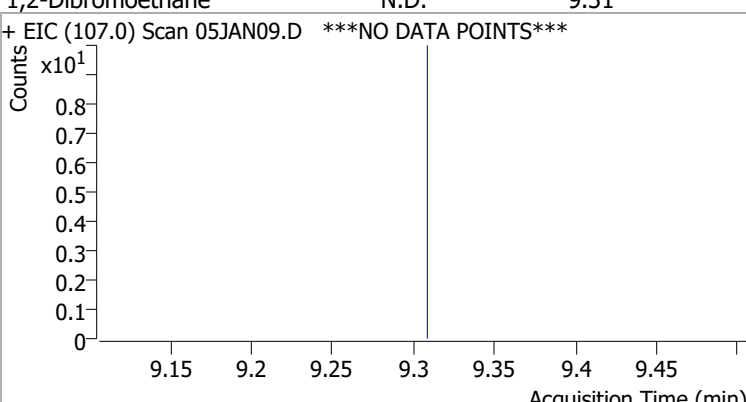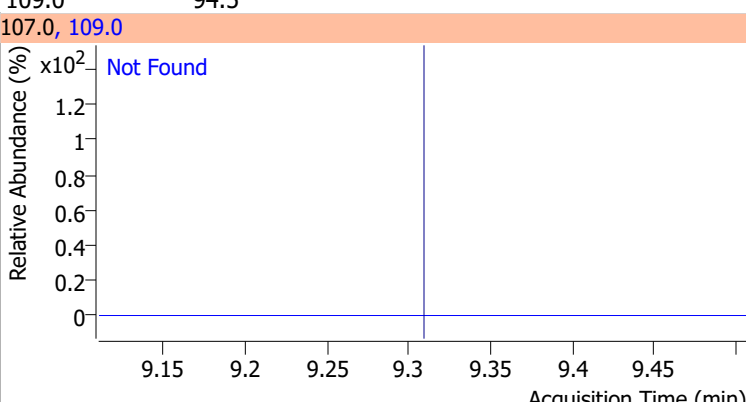
| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--|-------|--------|--|-----------|-------|-----------|
| Tetrachloroethene | N.D. | 8.94 | 165.8 | 128.6 | 129.0 | 91.5 |
| + EIC (163.8) Scan 05JAN09.D ***NO DATA POINTS*** | | | 163.8, 129.0, 165.8 | | | |
|  | | |  | | | |
| 1,3-Dichloropropane | N.D. | 8.98 | 78.0 | 32.9 | | |
| + EIC (76.0) Scan 05JAN09.D | | | 76.0, 78.0 | | | |
|  | | |  | | | |
| Chlorodibromomethane | N.D. | 9.21 | 127.0 | 78.0 | | |
| + EIC (129.0) Scan 05JAN09.D | | | 129.0, 127.0 | | | |
|  | | |  | | | |
| 1,2-Dibromoethane | N.D. | 9.31 | 109.0 | 94.5 | | |
| + EIC (107.0) Scan 05JAN09.D ***NO DATA POINTS*** | | | 107.0, 109.0 | | | |
|  | | |  | | | |


Quantitation Results Report (QT Reviewed)
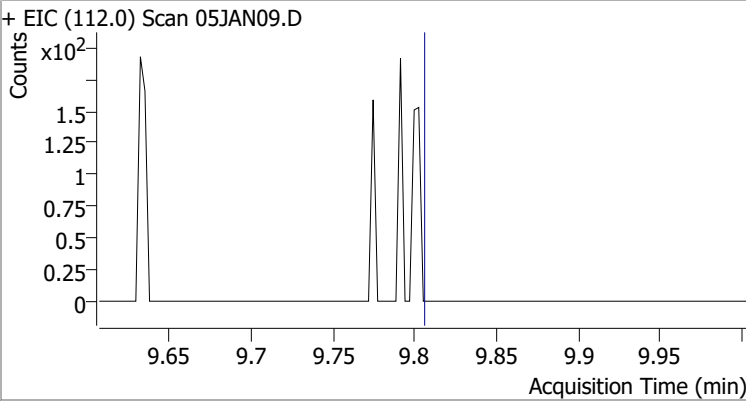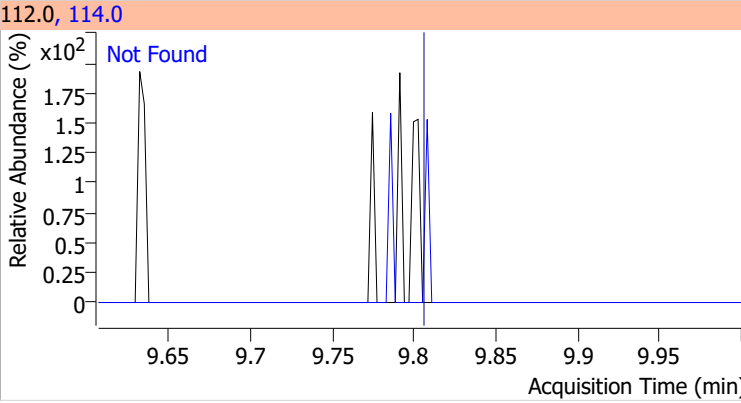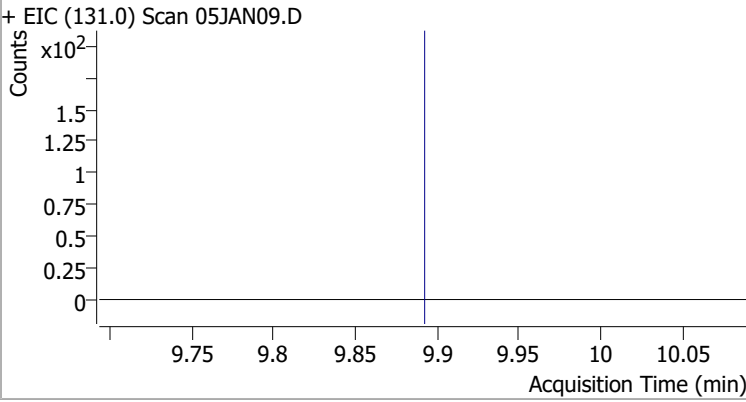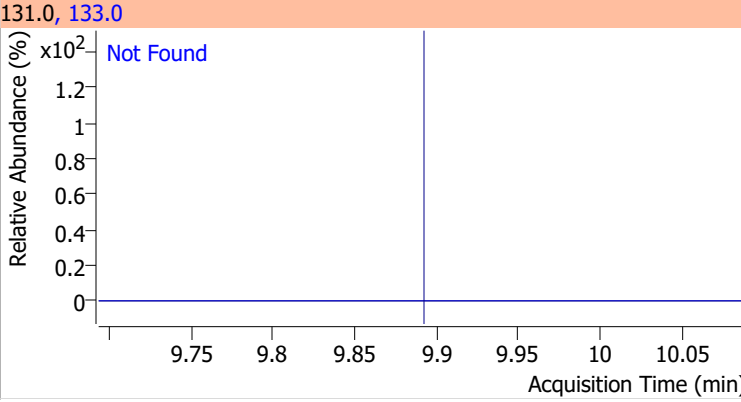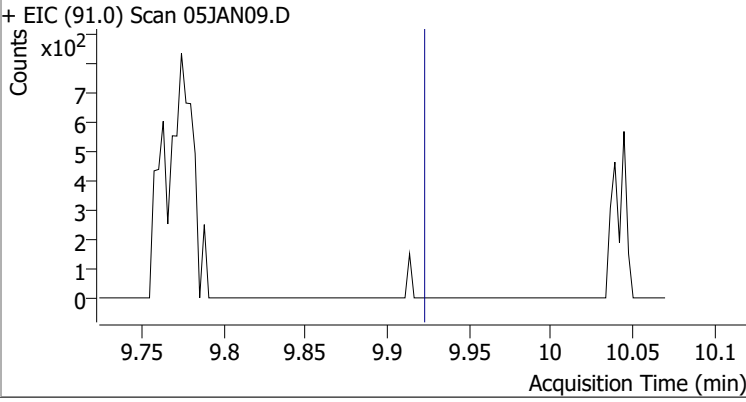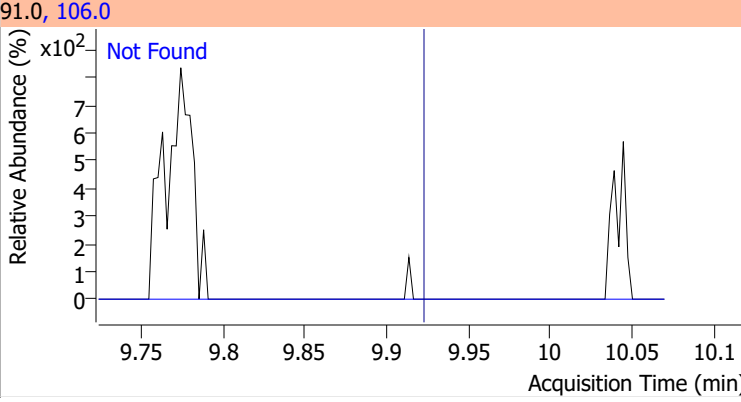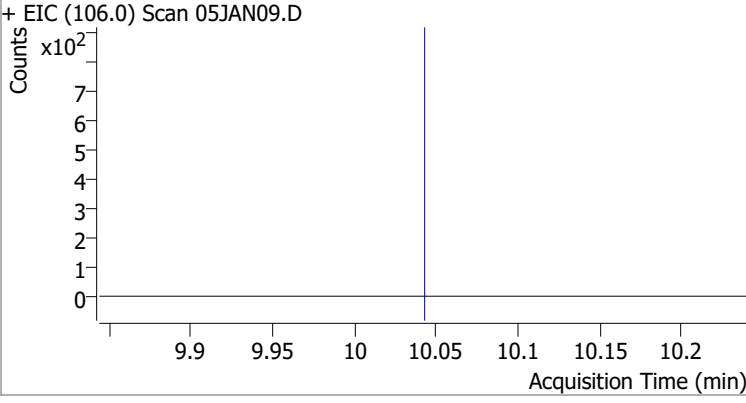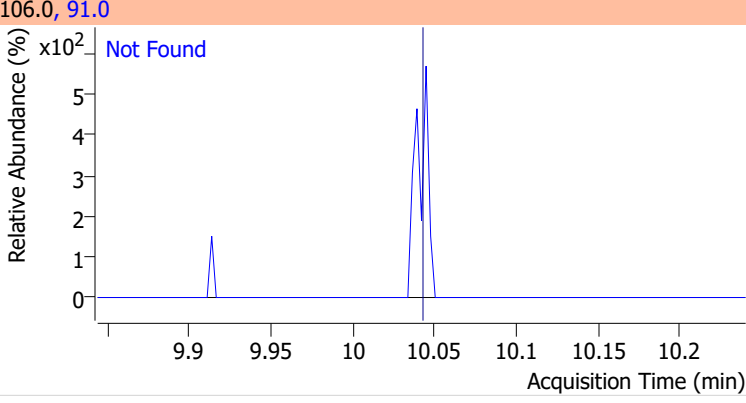
| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--|-------|--------|---|-----------|
| Chlorobenzene | N.D. | 9.80 | 114.0 | 32.1 |
| + EIC (112.0) Scan 05JAN09.D  | | | 112.0, 114.0  | |
| 1,1,1,2-Tetrachloroethane | N.D. | 9.89 | 133.0 | 98.6 |
| + EIC (131.0) Scan 05JAN09.D  | | | 131.0, 133.0  | |
| Ethylbenzene | N.D. | 9.92 | 106.0 | 31.1 |
| + EIC (91.0) Scan 05JAN09.D  | | | 91.0, 106.0  | |
| m+p-Xylenes | N.D. | 10.04 | 91.0 | 201.4 |
| + EIC (106.0) Scan 05JAN09.D  | | | 106.0, 91.0  | |

Quantitation Results Report (QT Reviewed)

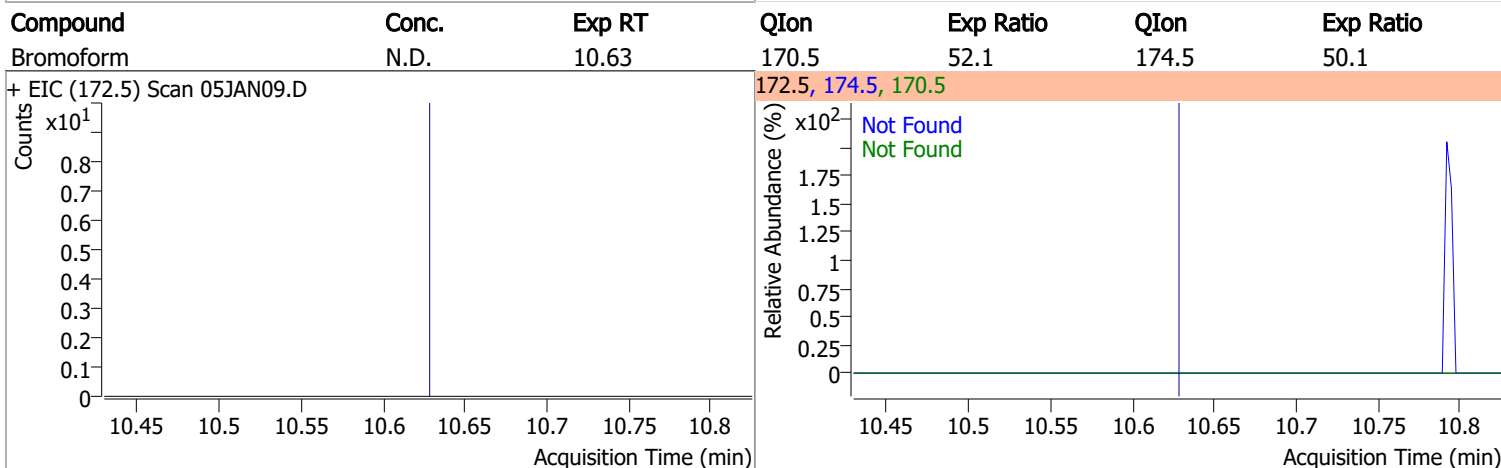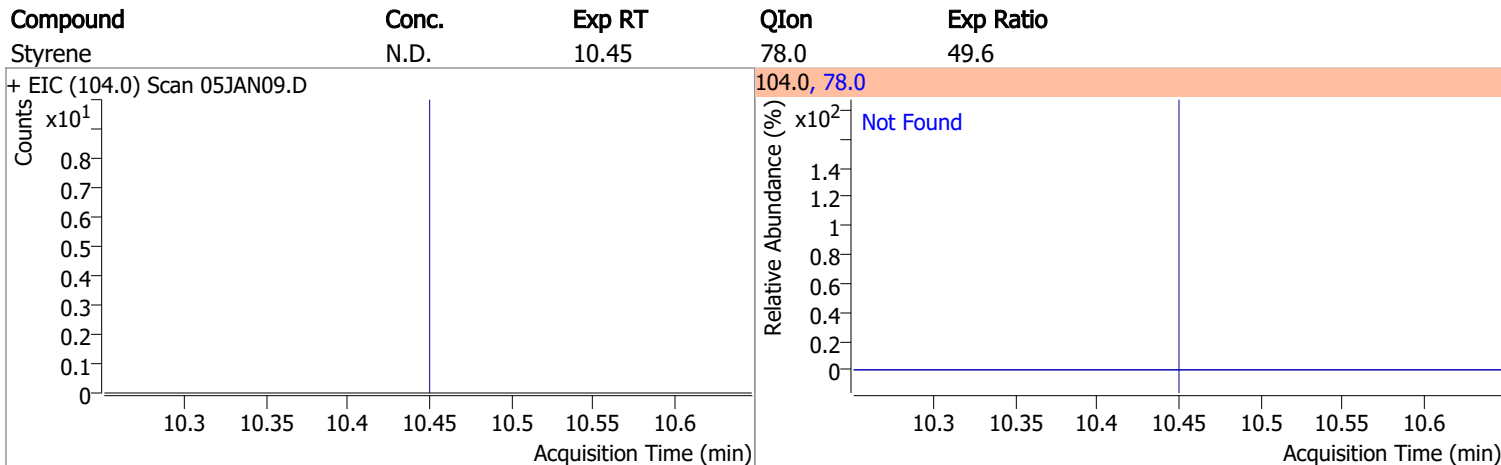


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 268.5403 | 10.95 | 0.00 | 214927 | 174.0 | 93.3 | 61.7 | 121.7 |
| | | | | | 176.0 | 91.5 | 60.6 | 120.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------|-------|--------|------|-----------|-------|-----------|
| Bromobenzene | N.D. | 11.09 | 77.0 | 145.7 | 158.0 | 96.5 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------------|-------|--------|------|-----------|
| 1,1,2,2-Tetrachloroethane | N.D. | 11.12 | 85.0 | 66.2 |











| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|------------------------|-------|--------|-------|-----------|
| 1,2,3-Trichloropropane | N.D. | 11.15 | 112.0 | 63.5 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|-----------------|-------|--------|------|-----------|
| 2-Chlorotoluene | N.D. | 11.29 | 91.0 | 282.3 |




Quantitation Results Report (QT Reviewed)
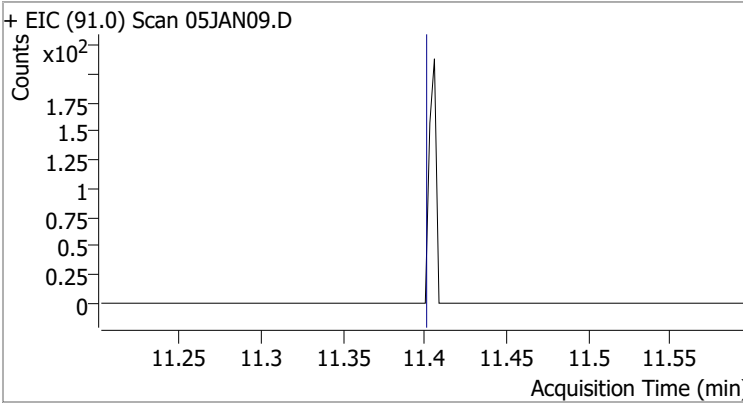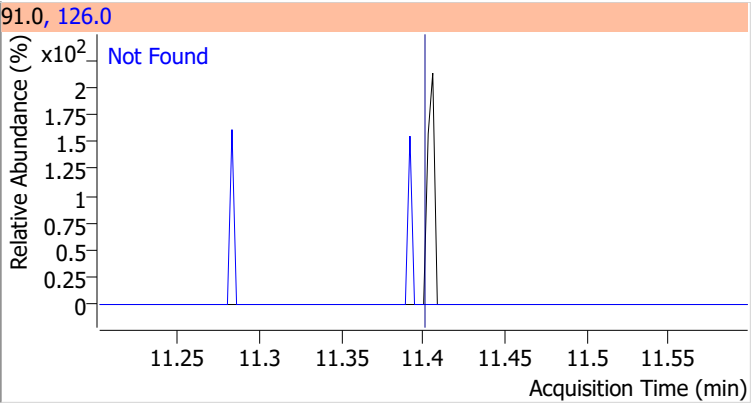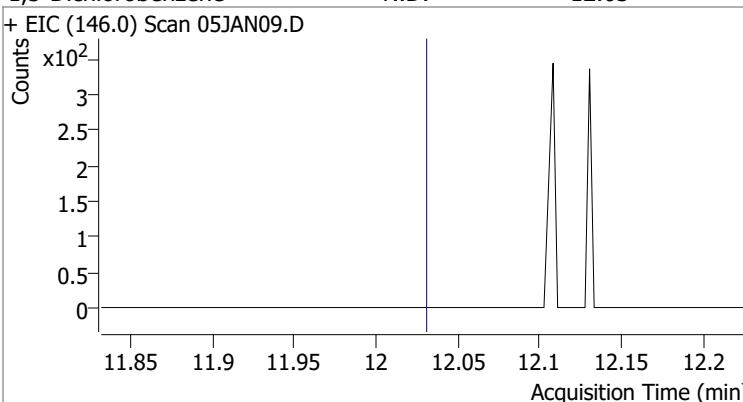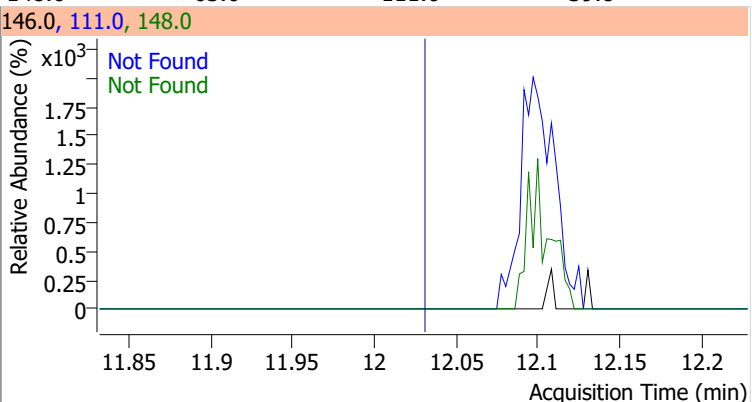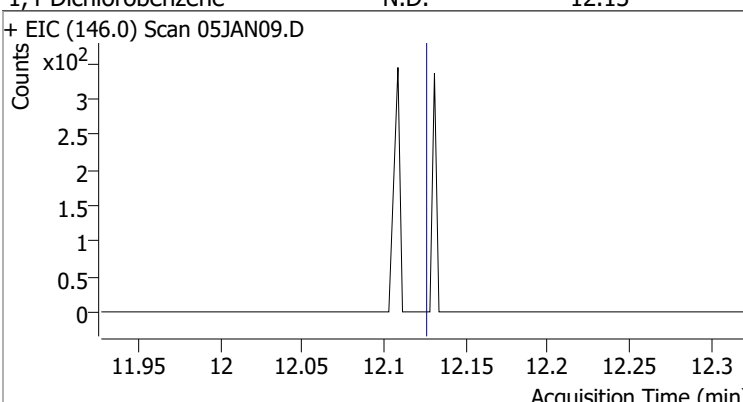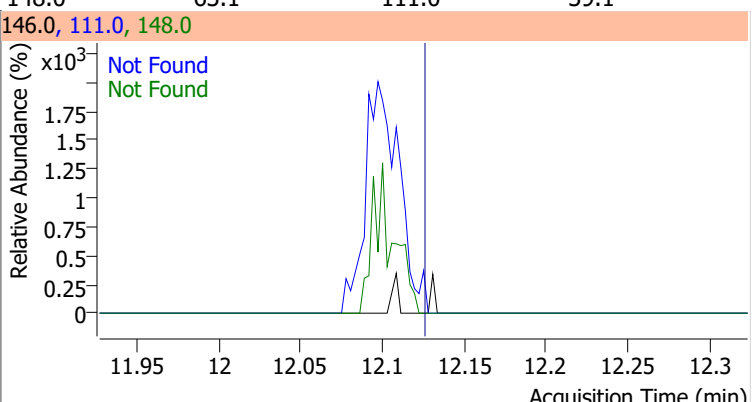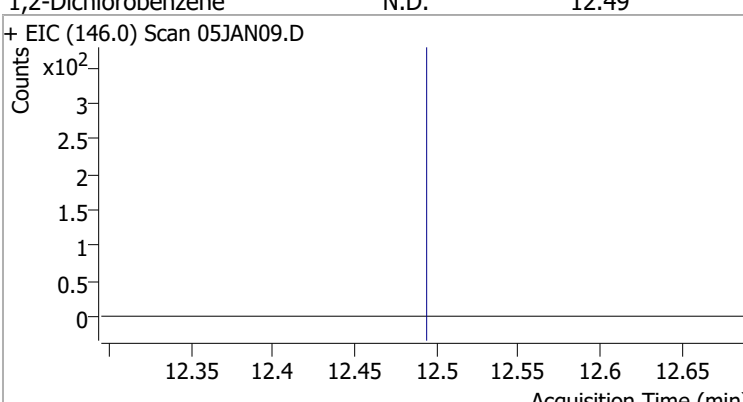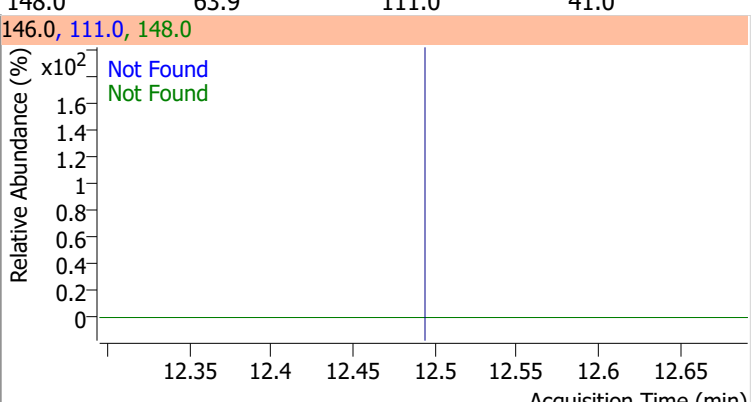
| Compound | Conc. | Exp RT | QIon | Exp Ratio | | | | |
|--|-------|--------|--|-----------|------|-----------|--|--|
| 4-Chlorotoluene | N.D. | 11.40 | 126.0 | 31.7 | | | | |
| + EIC (91.0) Scan 05JAN09.D | | | 91.0, 126.0 | | | | | |
|  | | |  | | | | | |
| 1,3-Dichlorobenzene | N.D. | 12.03 | 148.0 | 63.6 | QIon | Exp Ratio | | |
| + EIC (146.0) Scan 05JAN09.D | | | 146.0, 111.0, 148.0 | | | | | |
|  | | |  | | | | | |
| 1,4-Dichlorobenzene | N.D. | 12.13 | 148.0 | 63.1 | QIon | Exp Ratio | | |
| + EIC (146.0) Scan 05JAN09.D | | | 146.0, 111.0, 148.0 | | | | | |
|  | | |  | | | | | |
| 1,2-Dichlorobenzene | N.D. | 12.49 | 148.0 | 63.9 | QIon | Exp Ratio | | |
| + EIC (146.0) Scan 05JAN09.D | | | 146.0, 111.0, 148.0 | | | | | |
|  | | |  | | | | | |

Quantitation Results Report (QT Reviewed)

| | | | |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File | 05JAN10.D | Operator | MSC |
| Acq. Method | 5975CACQF.M | Acq. Date-Time | 1/5/2022 2:11:00 PM |
| Sample Name | B22010134-002A | Instrument | VOA5975C |
| Vial | 10 | Multiplier | 1.00 |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m | Comment | |
| Tune File | BFB_Atune3.u | Tune Date | 10/11/2021 4:02:00 PM |
| Batch Name | VG010522_8260B.batch.bin | Last Calib Update | 2/28/2022 2:48:47 PM |
| Ref Library | \\MASSHUNTER\Org\Library\NIST129K.I | | |



| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|--------------------|-------|----------|
| Internal Standards | | | | | | |
| M Fluorobenzene | 6.618 | 96.0 | 727308 | 250.0000 | ng | -0.006 |
| M Chlorobenzene-d5 | 9.772 | 82.0 | 281773 | 250.0000 | ng | 0.000 |
| M 1,4-Dichlorobenzene-d4 | 12.100 | 152.0 | 213658 | 250.0000 | ng | 0.000 |
| System Monitoring Compounds | | | | | | |
| S Dibromofluoromethane | 5.845 | 113.0 | 192021 | 280.2417 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 80.0 - 119.0% | | | Recovery = 112.10% | | |
| S 1,2-Dichloroethane-d4 | 6.233 | 67.0 | 84898 | 286.8601 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 81.0 - 118.0% | | | Recovery = 114.74% | | |
| S Toluene-d8 | 8.319 | 98.0 | 729899 | 268.8089 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 89.0 - 112.0% | | | Recovery = 107.52% | | |
| S p-Bromofluorobenzene | 10.951 | 95.0 | 215264 | 275.0138 | ng | -0.003 |
| Spiked Amount: 250.000 | Range: 85.0 - 114.0% | | | Recovery = 110.01% | | |
| Target Compounds | | | | | | |
| T Dichlorodifluoromethane | 0.000 | | 0 | N.D. | | |
| T Chloromethane | 1.409 | 50.0 | 1273 | 1.1003 | ng | m 85 |
| T Vinyl chloride | 0.000 | | 0 | N.D. | | |
| T Bromomethane | 0.000 | | 0 | N.D. | | |
| T Chloroethane | 0.000 | | 0 | N.D. | | |
| T Trichlorofluoromethane | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methylene chloride | 3.338 | 49.0 | 1248 | 1.1560 | ng | m 83 |
| T trans-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methyl tert-butyl ether (MTBE) | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloroethane | 0.000 | | 0 | N.D. | | |
| T 2,2-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T cis-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methyl ethyl ketone | 0.000 | | 0 | N.D. | | |
| T Bromochloromethane | 0.000 | | 0 | N.D. | | |
| T Chloroform | 0.000 | | 0 | N.D. | | |


Quantitation Results Report (QT Reviewed)

| Compound | RT | QIon | Resp. | Conc. | Units | | Dev(Min) |
|-----------------------------|--------|-------|-------|--------|-------|----|----------|
| T 1,1,1-Trichloroethane | 0.000 | | 0 | N.D. | | | |
| T Carbon tetrachloride | 0.000 | | 0 | N.D. | | | |
| T 1,1-Dichloropropene | 0.000 | | 0 | N.D. | | | |
| T Benzene | 0.000 | | 0 | N.D. | | | |
| T 1,2-Dichloroethane | 0.000 | | 0 | N.D. | | | |
| T Trichloroethene | 0.000 | | 0 | N.D. | | | |
| T 1,2-Dichloropropane | 0.000 | | 0 | N.D. | | | |
| T Dibromomethane | 0.000 | | 0 | N.D. | | | |
| T Bromodichloromethane | 0.000 | | 0 | N.D. | | | |
| T cis-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | | |
| T Toluene | 8.380 | 92.0 | 1581 | 0.8620 | ng | m | 99 |
| T trans-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | | |
| T 1,1,2-Trichloroethane | 0.000 | | 0 | N.D. | | | |
| T Tetrachloroethene | 0.000 | | 0 | N.D. | | | |
| T 1,3-Dichloropropane | 0.000 | | 0 | N.D. | | | |
| T Chlorodibromomethane | 0.000 | | 0 | N.D. | | | |
| T 1,2-Dibromoethane | 0.000 | | 0 | N.D. | | | |
| T Chlorobenzene | 0.000 | | 0 | N.D. | | | |
| T 1,1,1,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | | |
| T Ethylbenzene | 0.000 | | 0 | N.D. | | | |
| T m+p-Xylenes | 10.042 | 106.0 | 0 | | ng | md | 1 |
| T o-Xylene | 0.000 | | 0 | N.D. | | | |
| T Styrene | 0.000 | | 0 | N.D. | | | |
| T Bromoform | 0.000 | | 0 | N.D. | | | |
| T Bromobenzene | 0.000 | | 0 | N.D. | | | |
| T 1,1,2,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | | |
| T 1,2,3-Trichloropropane | 0.000 | | 0 | N.D. | | | |
| T 2-Chlorotoluene | 0.000 | | 0 | N.D. | | | |
| T 4-Chlorotoluene | 0.000 | | 0 | N.D. | | | |
| T 1,3-Dichlorobenzene | 0.000 | | 0 | N.D. | | | |
| T 1,4-Dichlorobenzene | 0.000 | | 0 | N.D. | | | |
| T 1,2-Dichlorobenzene | 0.000 | | 0 | N.D. | | | |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|-------------------------|-------|--------|------|-----------|
| Dichlorodifluoromethane | N.D. | 1.24 | 87.0 | 32.3 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------|--------|------|----------|----------|------|--------|-------|-------|
| Chloromethane | 1.1003 | 1.41 | 0.00 | 1273 (m) | 52.0 | 40.3 | 2.1 | 62.1 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------------|-------|--------|------|-----------|
| Vinyl chloride | N.D. | 1.50 | 64.0 | 29.9 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------|-------|--------|------|-----------|
| Bromomethane | N.D. | 1.80 | 94.0 | 104.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------|-------|--------|------|-----------|
| Chloroethane | N.D. | 1.89 | 66.0 | 30.1 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|------------------------|-------|--------|-------|-----------|
| Trichlorofluoromethane | N.D. | 2.14 | 103.0 | 64.2 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethene | N.D. | 2.70 | 61.0 | 180.3 | 63.0 | 56.7 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|--------|------|----------|----------|------|--------|-------|-------|
| Methylene chloride | 1.1560 | 3.34 | 0.00 | 1248 (m) | 84.0 | 54.5 | 36.9 | 96.9 |
| | | | | | 86.0 | 31.8 | 14.3 | 74.3 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,2-Dichloroethene | N.D. | 3.72 | 61.0 | 153.9 | 98.0 | 65.7 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------------------|-------|--------|------|-----------|
| Methyl tert-butyl ether (MTBE) | N.D. | 3.75 | 57.0 | 24.6 |







| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethane | N.D. | 4.38 | 65.0 | 32.1 | 83.0 | 13.7 |







| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|------|-----------|
| 2,2-Dichloropropane | N.D. | 5.20 | 41.0 | 66.5 | 97.0 | 23.2 |



Quantitation Results Report (QT Reviewed)

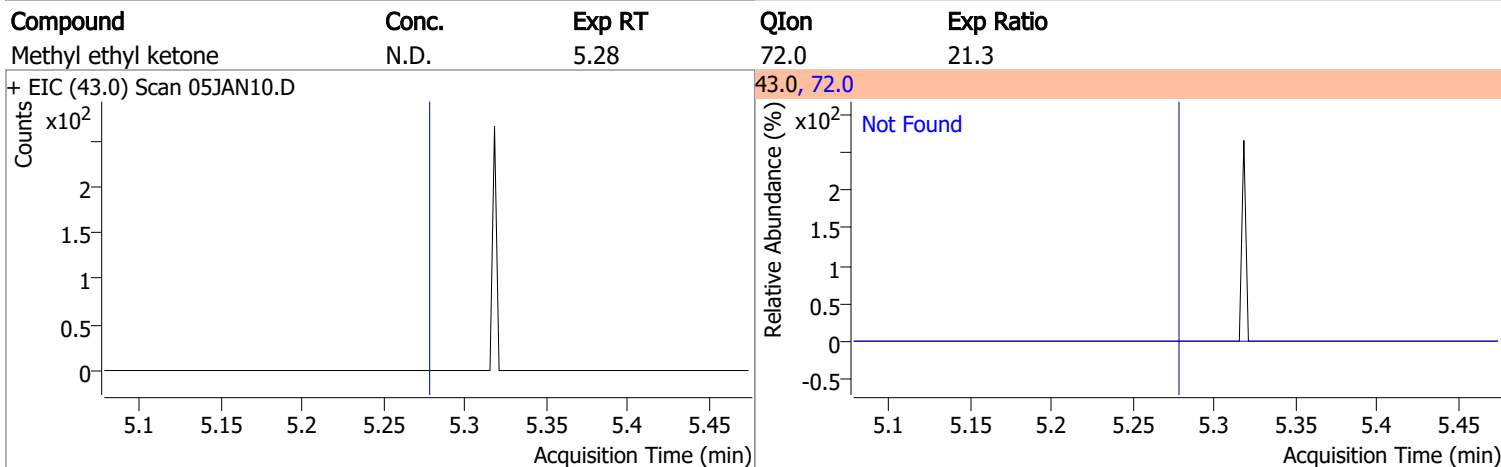


Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 286.8601 | 6.23 | 0.00 | 84898 | 65.0 | 197.0 | 166.5 | 226.5 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------|-------|--------|------|-----------|
| Benzene | N.D. | 6.28 | 77.0 | 23.5 |







| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,2-Dichloroethane | N.D. | 6.32 | 64.0 | 29.9 | 98.0 | 7.6 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------|-------|--------|-------|-----------|------|-----------|
| Trichloroethene | N.D. | 7.03 | 130.0 | 101.5 | 97.0 | 64.1 |




Quantitation Results Report (QT Reviewed)

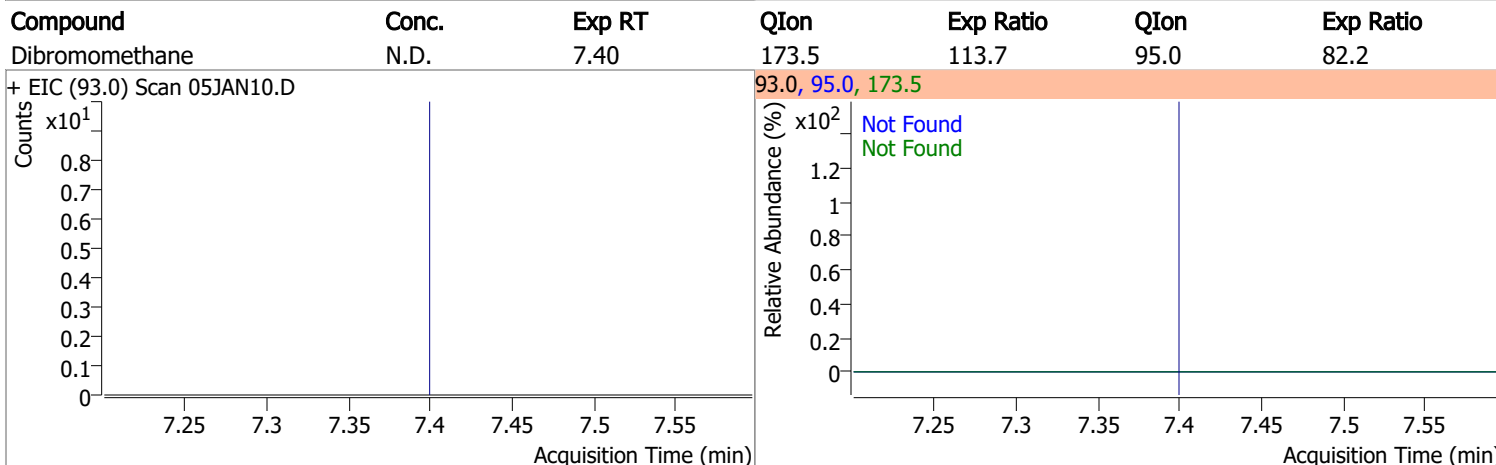


Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 268.8089 | 8.32 | 0.00 | 729899 | 100.0 | 64.4 | 34.4 | 94.4 |
| | | | | | 99.0 | 9.6 | 0.0 | 39.6 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|--------|------|----------|----------|------|--------|-------|-------|
| Toluene | 0.8620 | 8.38 | -0.01 | 1581 (m) | 91.0 | 174.3 | 145.8 | 205.8 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,3-Dichloropropene | N.D. | 8.64 | 39.0 | 53.4 | 77.0 | 32.4 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------------|-------|--------|------|-----------|------|-----------|
| 1,1,2-Trichloroethane | N.D. | 8.82 | 97.0 | 114.6 | 85.0 | 67.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-------------------|-------|--------|-------|-----------|-------|-----------|
| Tetrachloroethene | N.D. | 8.94 | 165.8 | 128.6 | 129.0 | 91.5 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| 1,3-Dichloropropane | N.D. | 8.98 | 78.0 | 32.9 |







| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------------------|-------|--------|-------|-----------|
| Chlorodibromomethane | N.D. | 9.21 | 127.0 | 78.0 |






| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|-------------------|-------|--------|-------|-----------|
| 1,2-Dibromoethane | N.D. | 9.31 | 109.0 | 94.5 |




Quantitation Results Report (QT Reviewed)

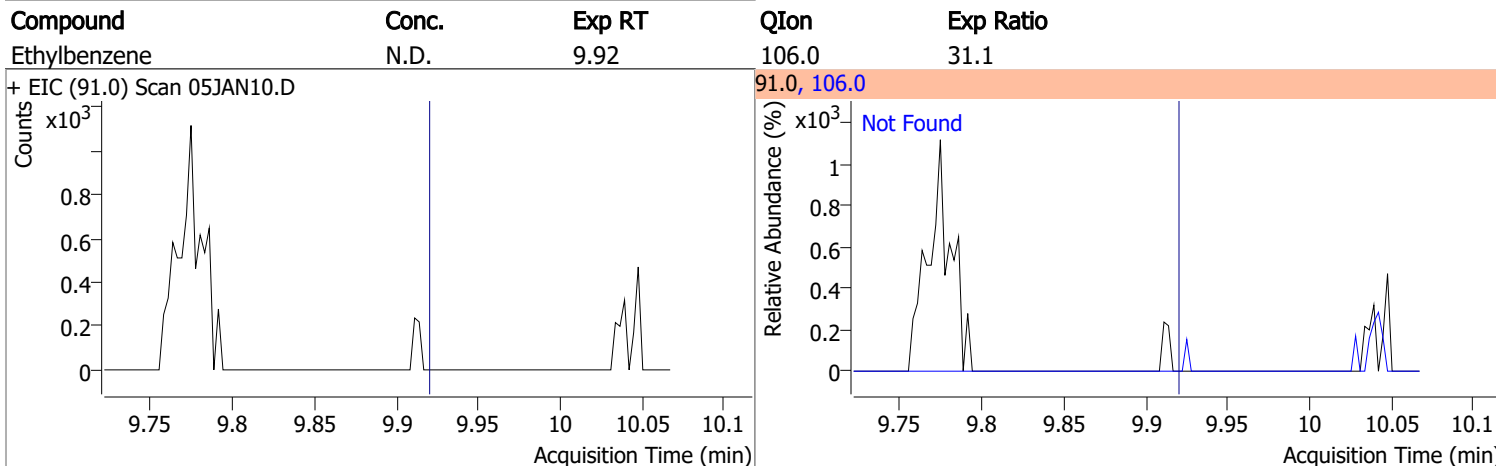









Quantitation Results Report (QT Reviewed)

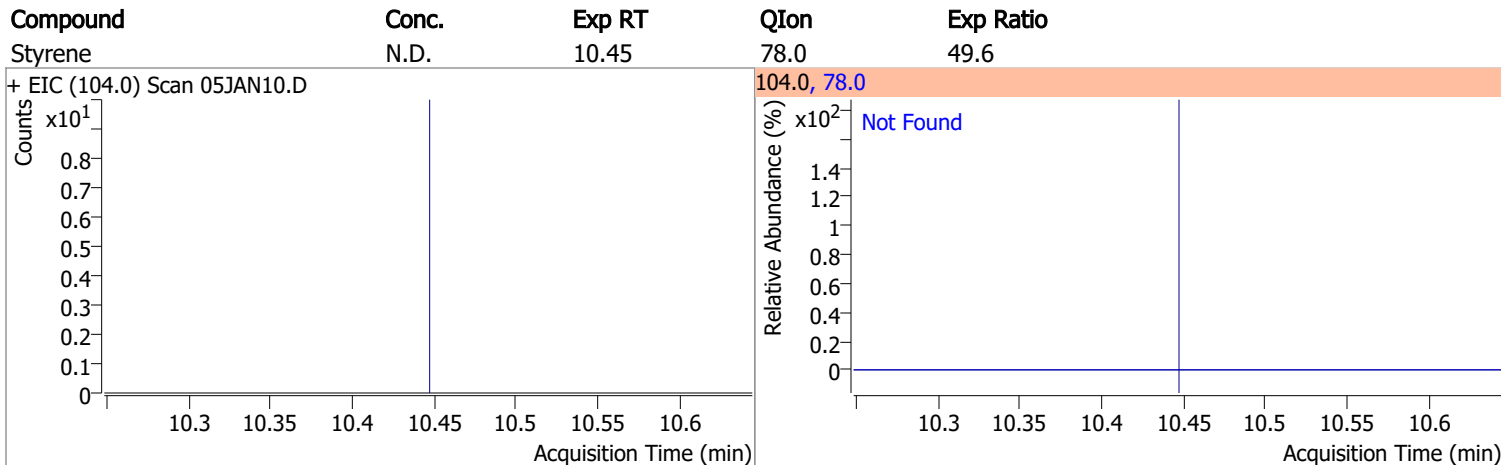









| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 275.0138 | 10.95 | 0.00 | 215264 | 174.0 | 93.1 | 61.7 | 121.7 |
| | | | | | 176.0 | 89.3 | 60.6 | 120.6 |



Quantitation Results Report (QT Reviewed)

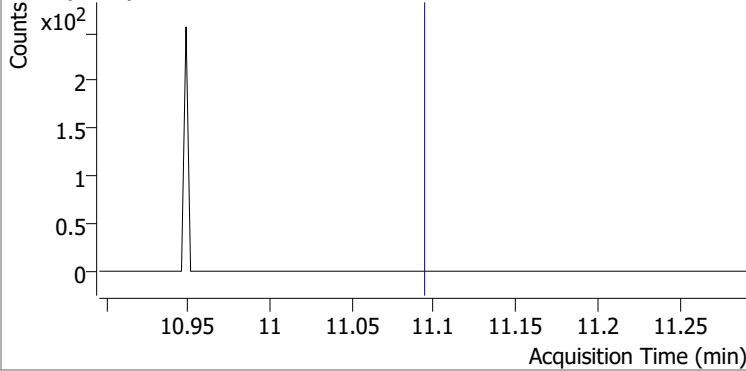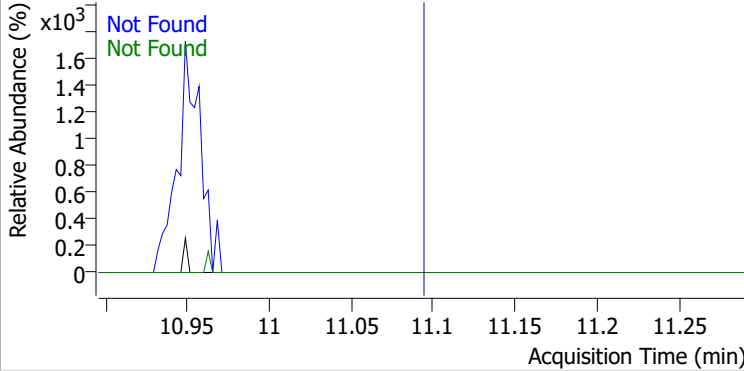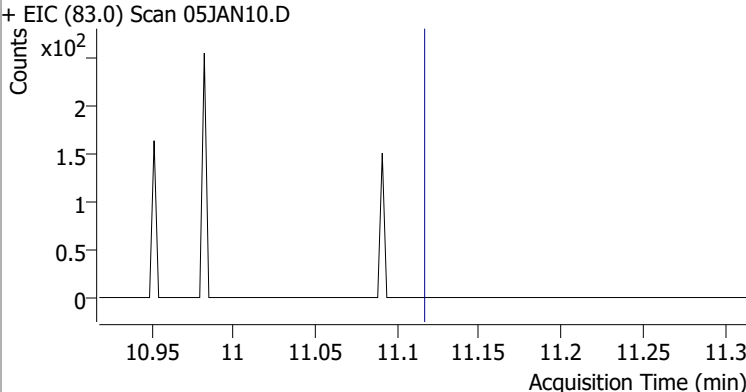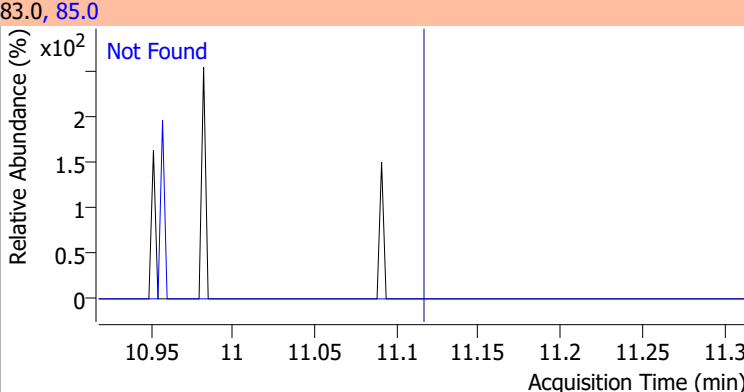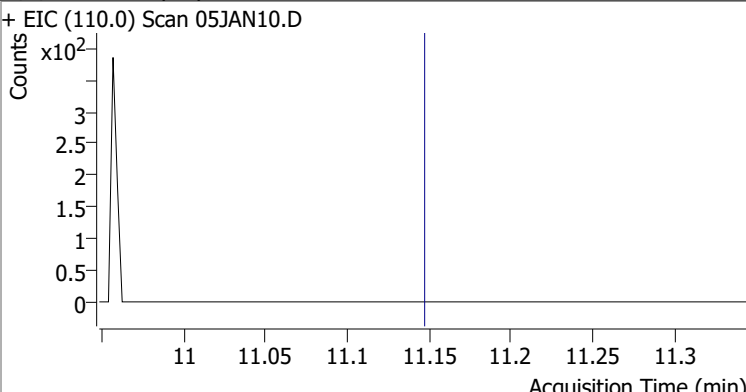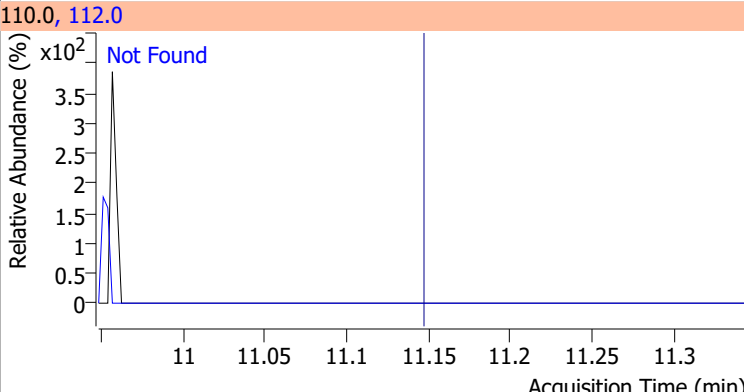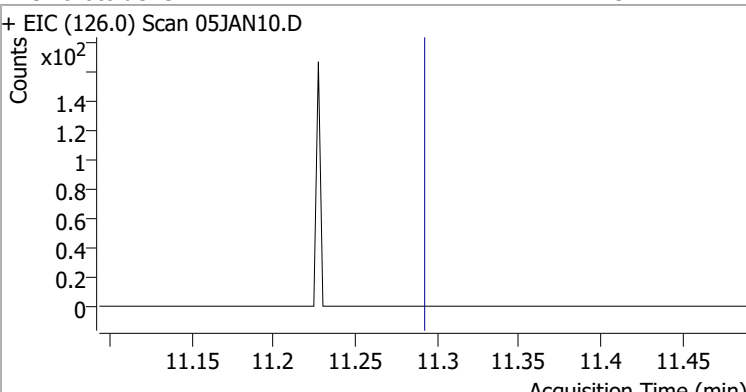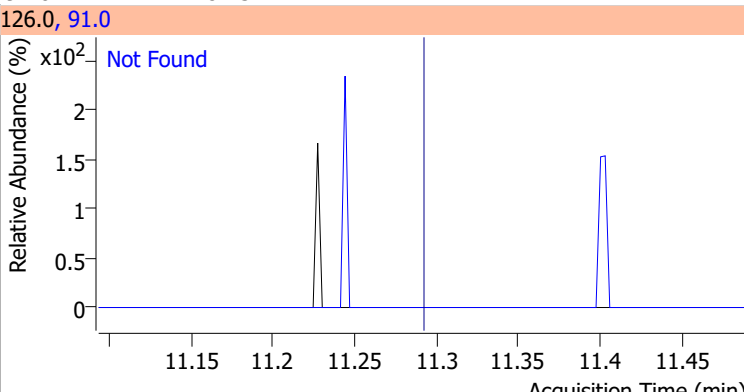
| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--|-------|--------|--|-----------|-------|-----------|
| Bromobenzene | N.D. | 11.09 | 77.0 | 145.7 | 158.0 | 96.5 |
| + EIC (156.0) Scan 05JAN10.D | | | 156.0, 77.0, 158.0 | | | |
|  | | |  | | | |
| 1,1,2-Tetrachloroethane | N.D. | 11.12 | 85.0 | 66.2 | | |
| + EIC (83.0) Scan 05JAN10.D | | | 83.0, 85.0 | | | |
|  | | |  | | | |
| 1,2,3-Trichloropropane | N.D. | 11.15 | 112.0 | 63.5 | | |
| + EIC (110.0) Scan 05JAN10.D | | | 110.0, 112.0 | | | |
|  | | |  | | | |
| 2-Chlorotoluene | N.D. | 11.29 | 91.0 | 282.3 | | |
| + EIC (126.0) Scan 05JAN10.D | | | 126.0, 91.0 | | | |
|  | | |  | | | |

Quantitation Results Report (QT Reviewed)
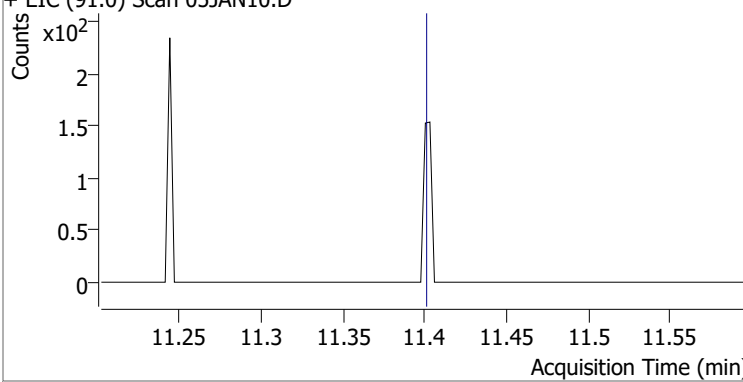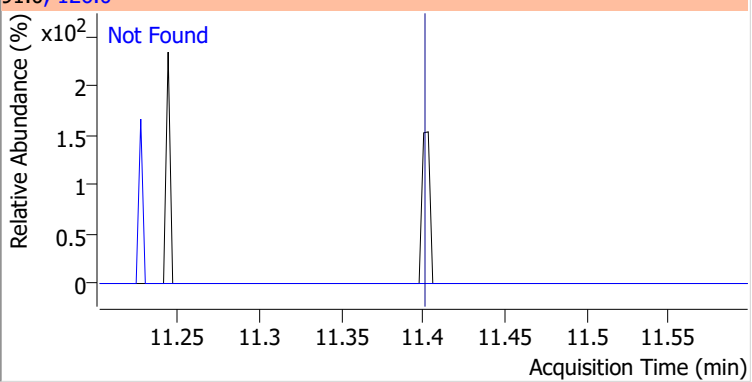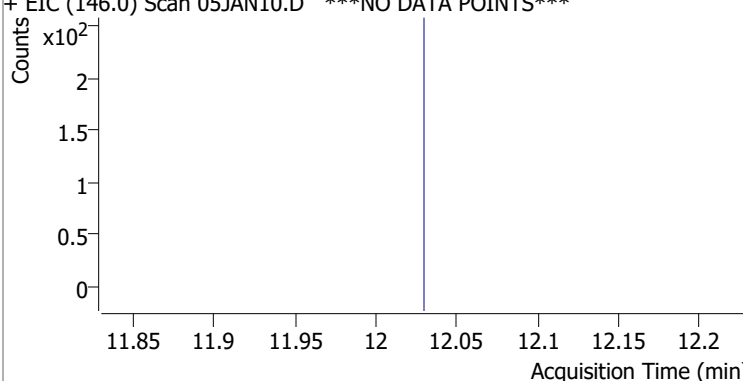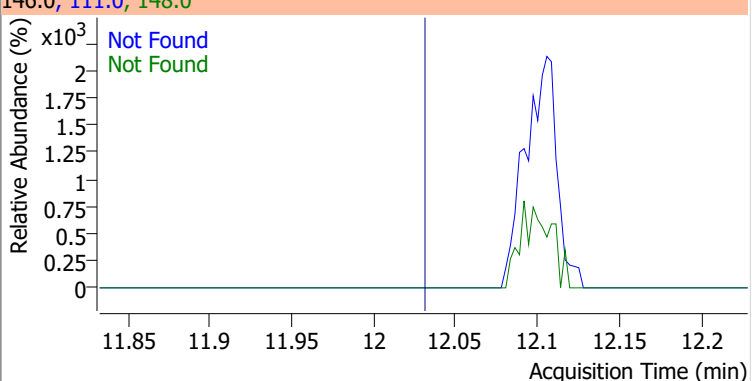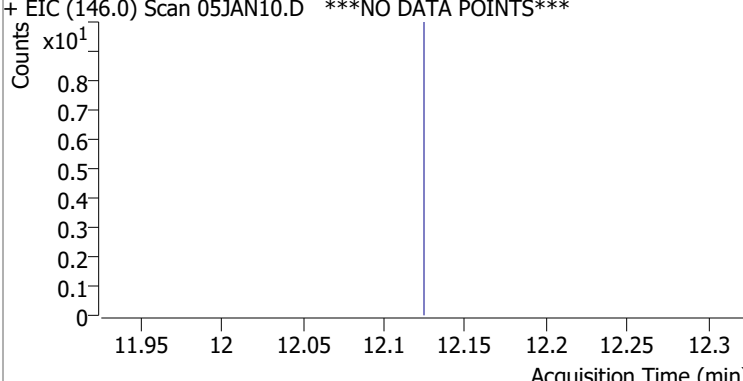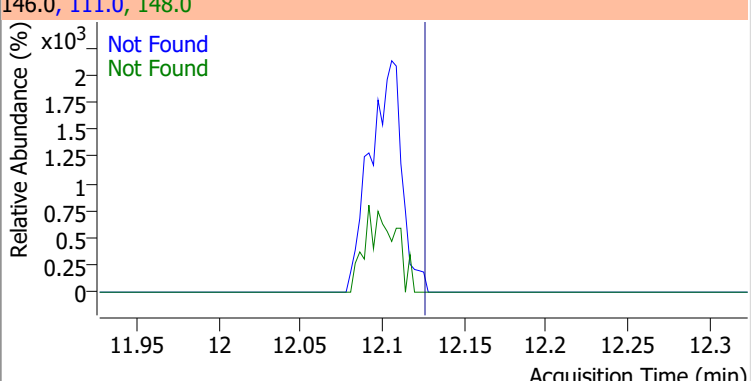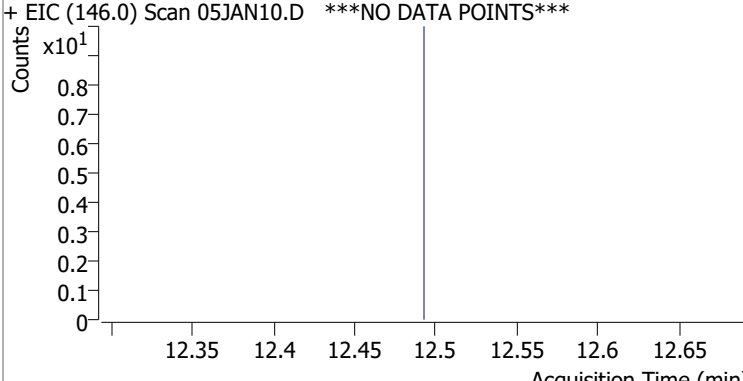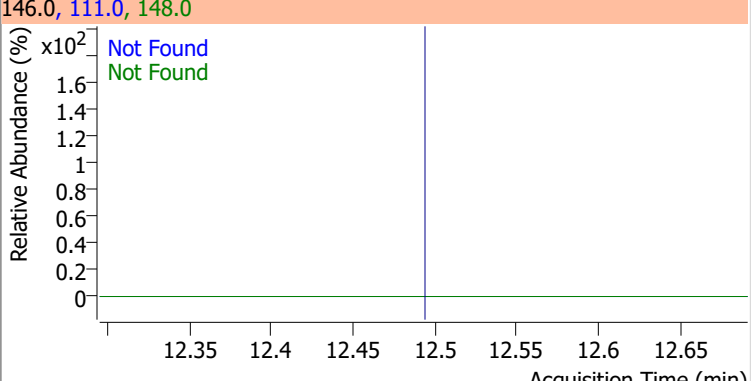
| Compound | Conc. | Exp RT | QIon | Exp Ratio | | |
|--|-------|--------|--|-----------|------|-----------|
| 4-Chlorotoluene | N.D. | 11.40 | 126.0 | 31.7 | | |
| + EIC (91.0) Scan 05JAN10.D | | | 91.0, 126.0 | | | |
|  | | |  | | | |
| 1,3-Dichlorobenzene | N.D. | 12.03 | 148.0 | 63.6 | QIon | Exp Ratio |
| + EIC (146.0) Scan 05JAN10.D ***NO DATA POINTS*** | | | 146.0, 111.0, 148.0 | | | |
|  | | |  | | | |
| 1,4-Dichlorobenzene | N.D. | 12.13 | 148.0 | 63.1 | QIon | Exp Ratio |
| + EIC (146.0) Scan 05JAN10.D ***NO DATA POINTS*** | | | 146.0, 111.0, 148.0 | | | |
|  | | |  | | | |
| 1,2-Dichlorobenzene | N.D. | 12.49 | 148.0 | 63.9 | QIon | Exp Ratio |
| + EIC (146.0) Scan 05JAN10.D ***NO DATA POINTS*** | | | 146.0, 111.0, 148.0 | | | |
|  | | |  | | | |

Quantitation Results Report (QT Reviewed)

| | | | |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File | 05JAN11.D | Operator | MSC |
| Acq. Method | 5975CACQF.M | Acq. Date-Time | 1/5/2022 2:38:23 PM |
| Sample Name | B22010141-002A | Instrument | VOA5975C |
| Vial | 11 | Multiplier | 1.00 |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m | Comment | |
| Tune File | BFB_Atune3.u | Tune Date | 10/11/2021 4:02:00 PM |
| Batch Name | VG010522_8260B.batch.bin | Last Calib Update | 2/28/2022 2:48:47 PM |
| Ref Library | \\MASSHUNTER\Org\Library\NIST129K.I | | |



| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|--------------------|-------|----------|
| Internal Standards | | | | | | |
| M Fluorobenzene | 6.621 | 96.0 | 721833 | 250.0000 | ng | -0.003 |
| M Chlorobenzene-d5 | 9.774 | 82.0 | 281916 | 250.0000 | ng | 0.003 |
| M 1,4-Dichlorobenzene-d4 | 12.100 | 152.0 | 214566 | 250.0000 | ng | 0.000 |
| System Monitoring Compounds | | | | | | |
| S Dibromofluoromethane | 5.848 | 113.0 | 190628 | 280.3188 | ng | 0.003 |
| Spiked Amount: 250.000 | Range: 80.0 - 119.0% | | | Recovery = 112.13% | | |
| S 1,2-Dichloroethane-d4 | 6.233 | 67.0 | 85616 | 291.4804 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 81.0 - 118.0% | | | Recovery = 116.59% | | |
| S Toluene-d8 | 8.322 | 98.0 | 727431 | 267.7641 | ng | 0.003 |
| Spiked Amount: 250.000 | Range: 89.0 - 112.0% | | | Recovery = 107.11% | | |
| S p-Bromofluorobenzene | 10.951 | 95.0 | 212552 | 270.3999 | ng | -0.003 |
| Spiked Amount: 250.000 | Range: 85.0 - 114.0% | | | Recovery = 108.16% | | |
| Target Compounds | | | | | | |
| T Dichlorodifluoromethane | 0.000 | | 0 | N.D. | | |
| T Chloromethane | 1.406 | 50.0 | 1466 | 1.2769 | ng | m 92 |
| T Vinyl chloride | 0.000 | | 0 | N.D. | | |
| T Bromomethane | 0.000 | | 0 | N.D. | | |
| T Chloroethane | 0.000 | | 0 | N.D. | | |
| T Trichlorofluoromethane | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methylene chloride | 3.335 | 49.0 | 1663 | 1.5517 | ng | m 90 |
| T trans-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methyl tert-butyl ether (MTBE) | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloroethane | 0.000 | | 0 | N.D. | | |
| T 2,2-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T cis-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methyl ethyl ketone | 0.000 | | 0 | N.D. | | |
| T Bromochloromethane | 0.000 | | 0 | N.D. | | |
| T Chloroform | 5.642 | 83.0 | 0 | | ng | md 1 |


Quantitation Results Report (QT Reviewed)

| Compound | RT | QIon | Resp. | Conc. | Units | | Dev(Min) |
|-----------------------------|--------|-------|-------|--------|-------|----|----------|
| T 1,1,1-Trichloroethane | 0.000 | | 0 | N.D. | | | |
| T Carbon tetrachloride | 0.000 | | 0 | N.D. | | | |
| T 1,1-Dichloropropene | 0.000 | | 0 | N.D. | | | |
| T Benzene | 6.272 | 78.0 | 424 | 0.1475 | ng | m | 93 |
| T 1,2-Dichloroethane | 0.000 | | 0 | N.D. | | | |
| T Trichloroethene | 0.000 | | 0 | N.D. | | | |
| T 1,2-Dichloropropane | 0.000 | | 0 | N.D. | | | |
| T Dibromomethane | 0.000 | | 0 | N.D. | | | |
| T Bromodichloromethane | 0.000 | | 0 | N.D. | | | |
| T cis-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | | |
| T Toluene | 8.386 | 92.0 | 2246 | 1.2239 | ng | | 97 |
| T trans-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | | |
| T 1,1,2-Trichloroethane | 0.000 | | 0 | N.D. | | | |
| T Tetrachloroethene | 0.000 | | 0 | N.D. | | | |
| T 1,3-Dichloropropane | 0.000 | | 0 | N.D. | | | |
| T Chlorodibromomethane | 0.000 | | 0 | N.D. | | | |
| T 1,2-Dibromoethane | 0.000 | | 0 | N.D. | | | |
| T Chlorobenzene | 0.000 | | 0 | N.D. | | | |
| T 1,1,1,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | | |
| T Ethylbenzene | 0.000 | | 0 | N.D. | | | |
| T m+p-Xylenes | 10.037 | 106.0 | 0 | | ng | md | 1 |
| T o-Xylene | 0.000 | | 0 | N.D. | | | |
| T Styrene | 0.000 | | 0 | N.D. | | | |
| T Bromoform | 0.000 | | 0 | N.D. | | | |
| T Bromobenzene | 0.000 | | 0 | N.D. | | | |
| T 1,1,2,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | | |
| T 1,2,3-Trichloropropane | 0.000 | | 0 | N.D. | | | |
| T 2-Chlorotoluene | 0.000 | | 0 | N.D. | | | |
| T 4-Chlorotoluene | 0.000 | | 0 | N.D. | | | |
| T 1,3-Dichlorobenzene | 0.000 | | 0 | N.D. | | | |
| T 1,4-Dichlorobenzene | 0.000 | | 0 | N.D. | | | |
| T 1,2-Dichlorobenzene | 0.000 | | 0 | N.D. | | | |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|-------------------------|-------|--------|------|-----------|
| Dichlorodifluoromethane | N.D. | 1.24 | 87.0 | 32.3 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------|--------|------|----------|----------|------|--------|-------|-------|
| Chloromethane | 1.2769 | 1.41 | 0.00 | 1466 (m) | 52.0 | 27.5 | 2.1 | 62.1 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------------|-------|--------|------|-----------|
| Vinyl chloride | N.D. | 1.50 | 64.0 | 29.9 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------|-------|--------|------|-----------|
| Bromomethane | N.D. | 1.80 | 94.0 | 104.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------|-------|--------|------|-----------|
| Chloroethane | N.D. | 1.89 | 66.0 | 30.1 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|------------------------|-------|--------|-------|-----------|
| Trichlorofluoromethane | N.D. | 2.14 | 103.0 | 64.2 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethene | N.D. | 2.70 | 61.0 | 180.3 | 63.0 | 56.7 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|--------|------|----------|----------|------|--------|-------|-------|
| Methylene chloride | 1.5517 | 3.34 | 0.00 | 1663 (m) | 84.0 | 76.8 | 36.9 | 96.9 |
| | | | | | 86.0 | 47.8 | 14.3 | 74.3 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,2-Dichloroethene | N.D. | 3.72 | 61.0 | 153.9 | 98.0 | 65.7 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------------------|-------|--------|------|-----------|
| Methyl tert-butyl ether (MTBE) | N.D. | 3.75 | 57.0 | 24.6 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethane | N.D. | 4.38 | 65.0 | 32.1 | 83.0 | 13.7 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|------|-----------|
| 2,2-Dichloropropane | N.D. | 5.20 | 41.0 | 66.5 | 97.0 | 23.2 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|------------------------|-------|--------|------|-----------|------|-----------|
| cis-1,2-Dichloroethene | N.D. | 5.22 | 61.0 | 167.2 | 98.0 | 67.3 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| Methyl ethyl ketone | N.D. | 5.28 | 72.0 | 21.3 |







| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|
| Bromochloromethane | N.D. | 5.52 | 49.0 | 182.9 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|-------|----|----------|-------|------|--------|-------|-------|
| Chloroform | | 0 | | 0 | 85.0 | | 36.0 | 96.0 |




Quantitation Results Report (QT Reviewed)

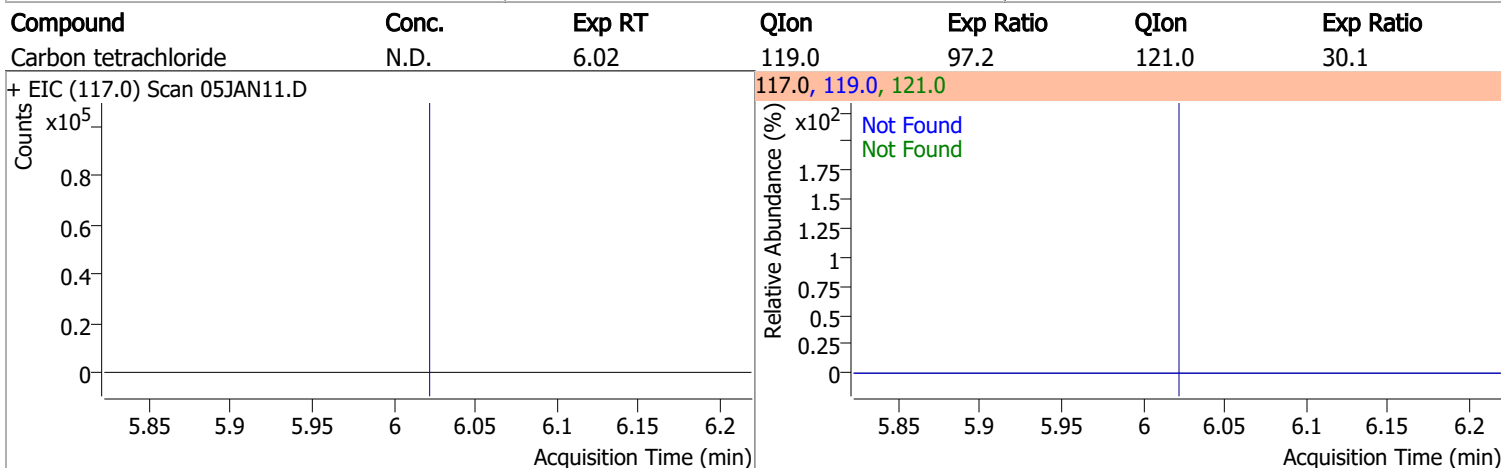


Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 291.4804 | 6.23 | 0.00 | 85616 | 65.0 | 195.9 | 166.5 | 226.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|--------|------|----------|---------|------|--------|-------|-------|
| Benzene | 0.1475 | 6.27 | -0.01 | 424 (m) | 77.0 | 19.9 | 0.0 | 53.5 |







| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,2-Dichloroethane | N.D. | 6.32 | 64.0 | 29.9 | 98.0 | 7.6 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------|-------|--------|-------|-----------|------|-----------|
| Trichloroethene | N.D. | 7.03 | 130.0 | 101.5 | 97.0 | 64.1 |




Quantitation Results Report (QT Reviewed)

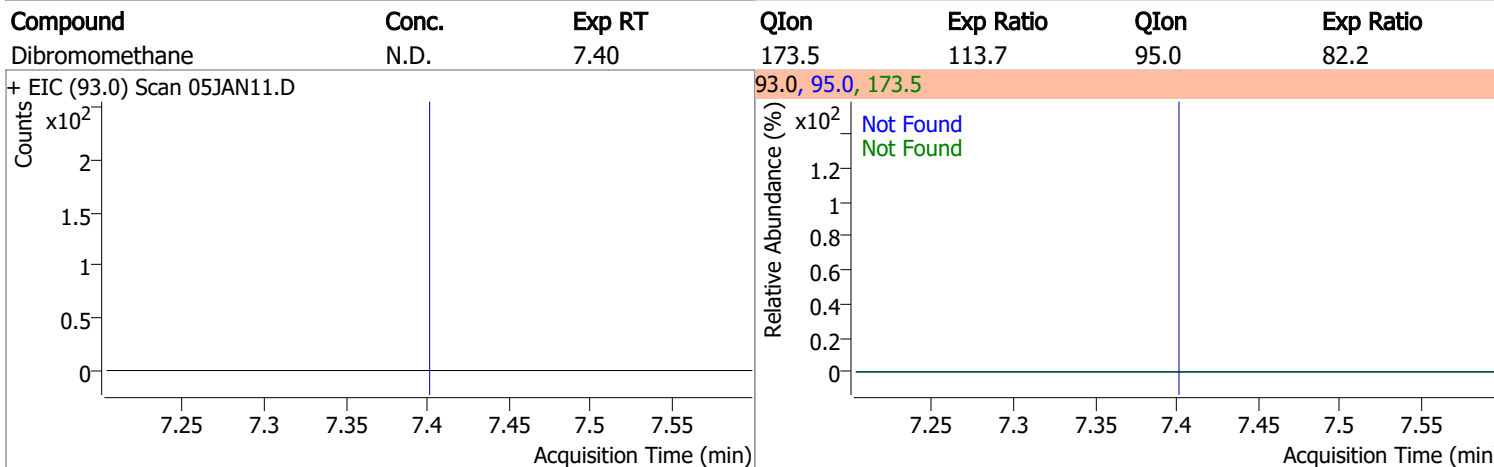


Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 267.7641 | 8.32 | 0.00 | 727431 | 100.0 | 64.2 | 34.4 | 94.4 |
| | | | | | 99.0 | 9.6 | 0.0 | 39.6 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|--------|------|----------|-------|------|--------|-------|-------|
| Toluene | 1.2239 | 8.39 | 0.00 | 2246 | 91.0 | 171.9 | 145.8 | 205.8 |











| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,3-Dichloropropene | N.D. | 8.64 | 39.0 | 53.4 | 77.0 | 32.4 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------------|-------|--------|------|-----------|------|-----------|
| 1,1,2-Trichloroethane | N.D. | 8.82 | 97.0 | 114.6 | 85.0 | 67.6 |




Quantitation Results Report (QT Reviewed)

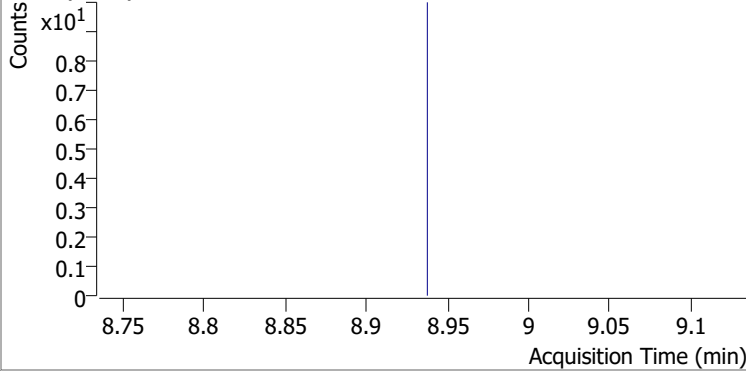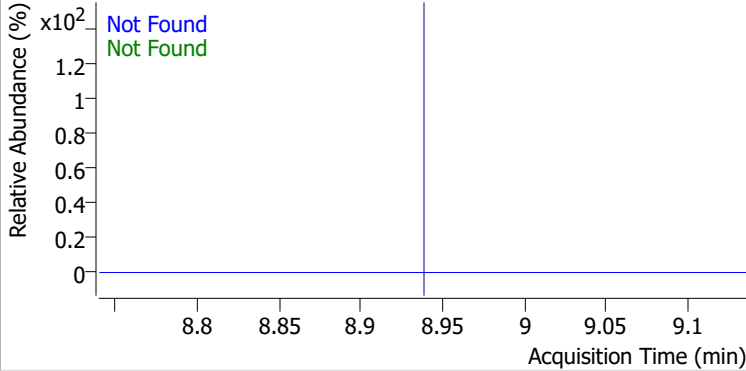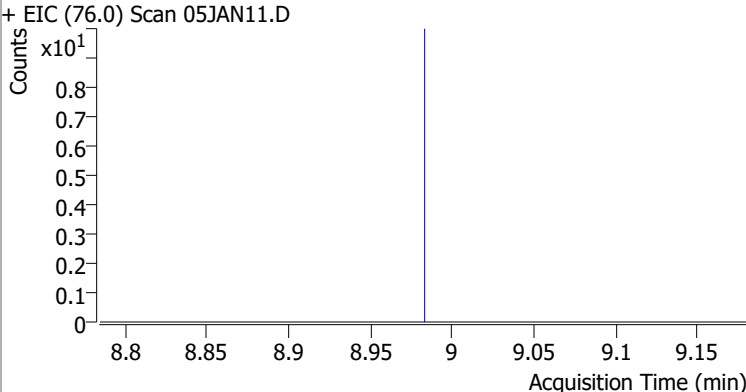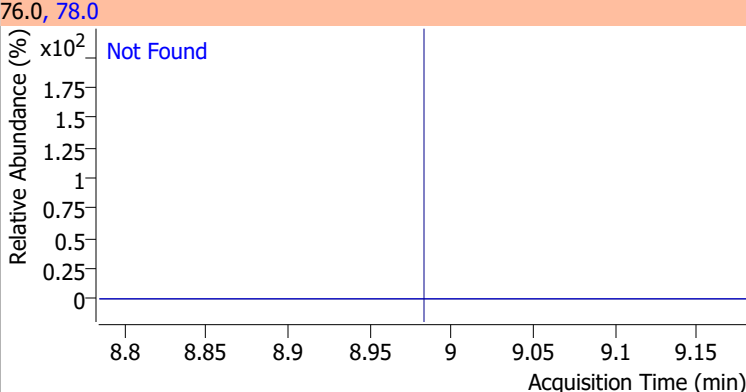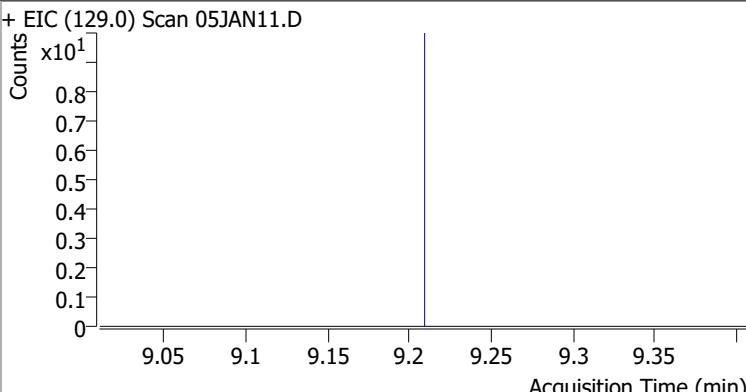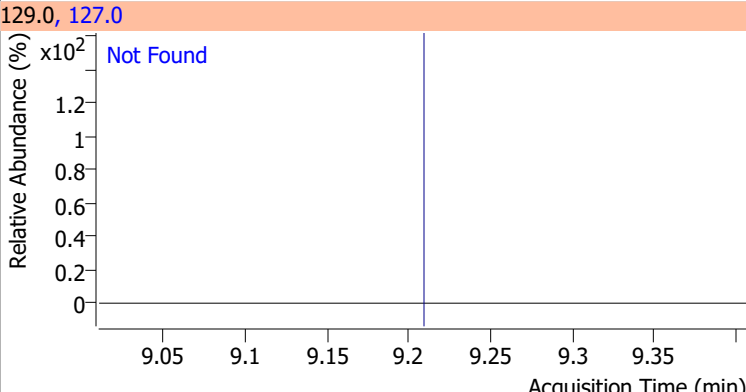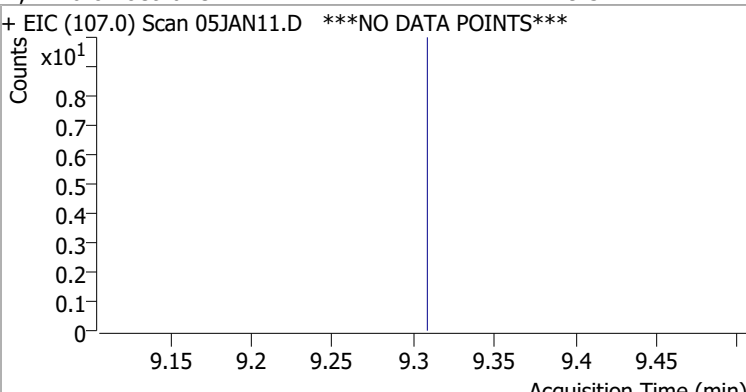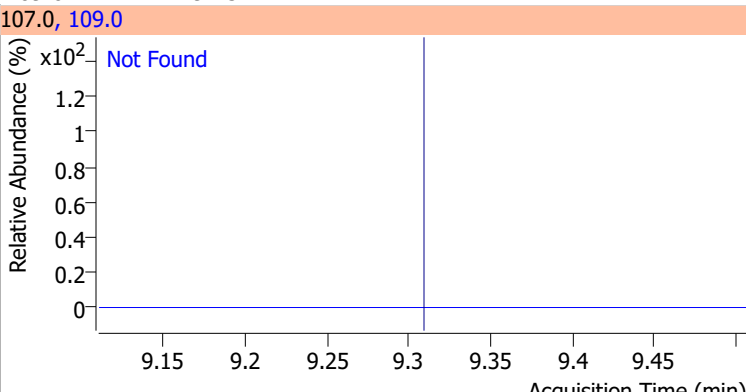
| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--|-------|--------|--|-----------|-------|-----------|
| Tetrachloroethene | N.D. | 8.94 | 165.8 | 128.6 | 129.0 | 91.5 |
| + EIC (163.8) Scan 05JAN11.D ***NO DATA POINTS*** | | | 163.8, 129.0, 165.8 | | | |
|  | | |  | | | |
| 1,3-Dichloropropane | N.D. | 8.98 | 78.0 | 32.9 | | |
| + EIC (76.0) Scan 05JAN11.D | | | 76.0, 78.0 | | | |
|  | | |  | | | |
| Chlorodibromomethane | N.D. | 9.21 | 127.0 | 78.0 | | |
| + EIC (129.0) Scan 05JAN11.D | | | 129.0, 127.0 | | | |
|  | | |  | | | |
| 1,2-Dibromoethane | N.D. | 9.31 | 109.0 | 94.5 | | |
| + EIC (107.0) Scan 05JAN11.D ***NO DATA POINTS*** | | | 107.0, 109.0 | | | |
|  | | |  | | | |

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------|-------|--------|-------|-----------|
| Chlorobenzene | N.D. | 9.80 | 114.0 | 32.1 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------------|-------|--------|-------|-----------|
| 1,1,1,2-Tetrachloroethane | N.D. | 9.89 | 133.0 | 98.6 |






| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------|-------|--------|-------|-----------|
| Ethylbenzene | N.D. | 9.92 | 106.0 | 31.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------|-------|----|----------|-------|------|--------|-------|-------|
| m+p-Xylenes | | 0 | | 0 | 91.0 | | 171.4 | 231.4 |











Quantitation Results Report (QT Reviewed)











| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 270.3999 | 10.95 | 0.00 | 212552 | 174.0 | 95.2 | 61.7 | 121.7 |
| | | | | | 176.0 | 92.3 | 60.6 | 120.6 |



Quantitation Results Report (QT Reviewed)

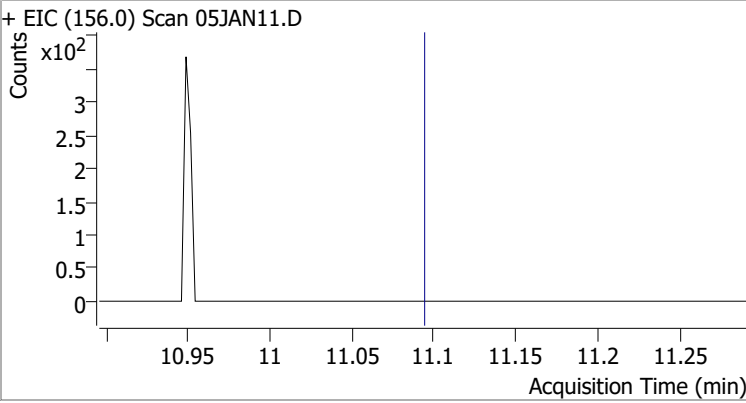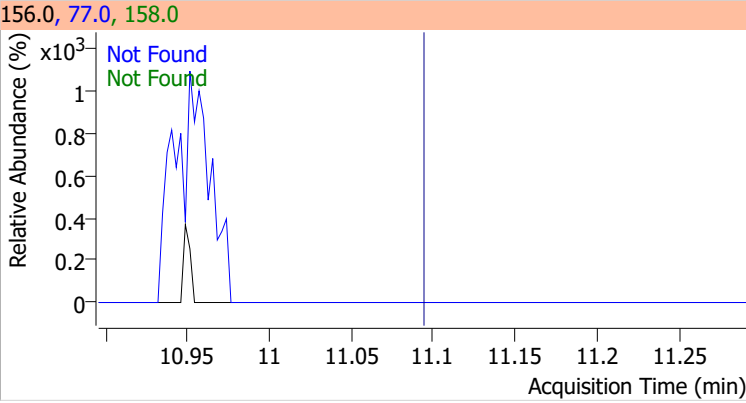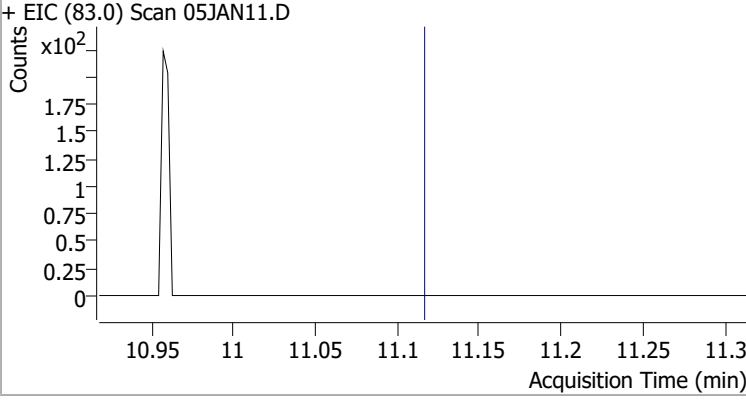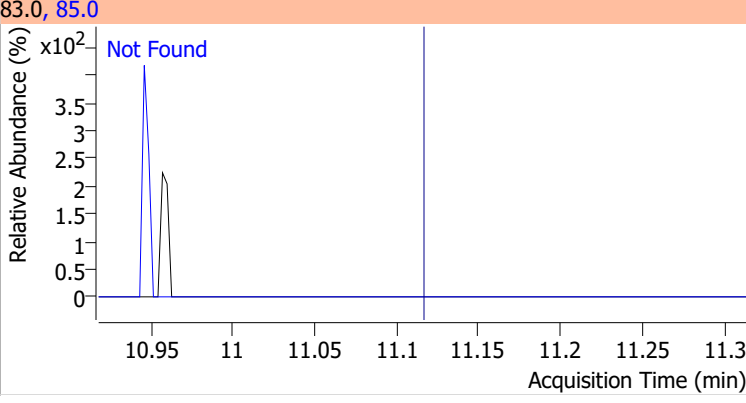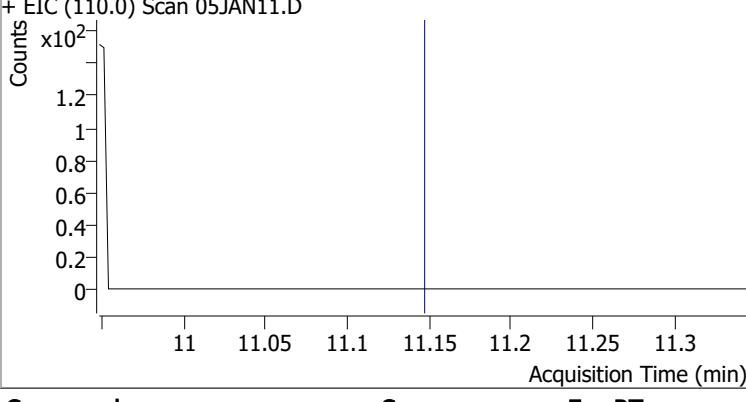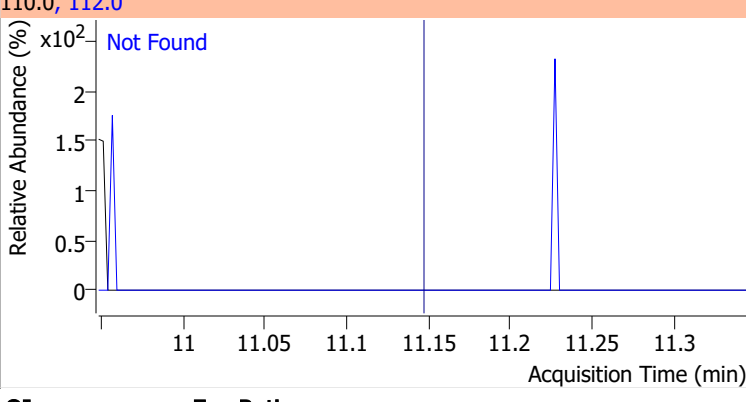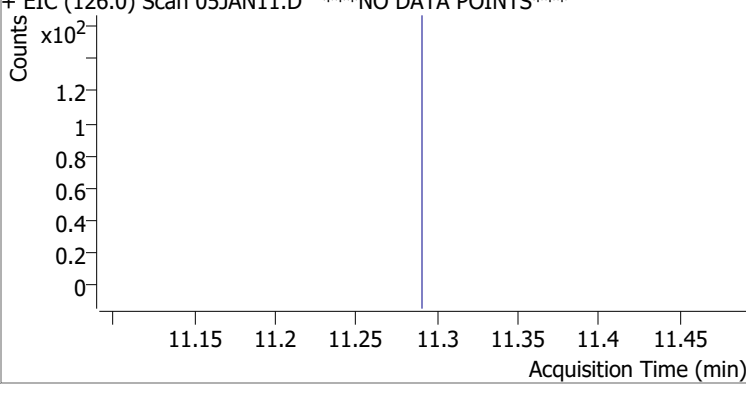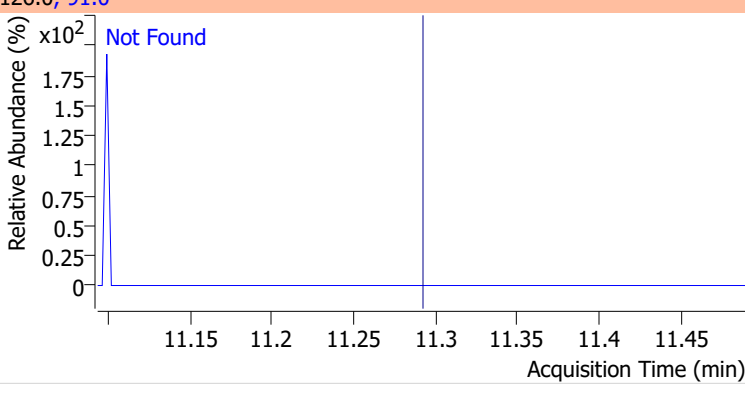
| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--|-------|--------|--|-----------|-------|-----------|
| Bromobenzene | N.D. | 11.09 | 77.0 | 145.7 | 158.0 | 96.5 |
| + EIC (156.0) Scan 05JAN11.D | | | 156.0, 77.0, 158.0 | | | |
|  | | |  | | | |
| 1,1,2,2-Tetrachloroethane | N.D. | 11.12 | 85.0 | 66.2 | | |
| + EIC (83.0) Scan 05JAN11.D | | | 83.0, 85.0 | | | |
|  | | |  | | | |
| 1,2,3-Trichloropropane | N.D. | 11.15 | 112.0 | 63.5 | | |
| + EIC (110.0) Scan 05JAN11.D | | | 110.0, 112.0 | | | |
|  | | |  | | | |
| 2-Chlorotoluene | N.D. | 11.29 | 91.0 | 282.3 | | |
| + EIC (126.0) Scan 05JAN11.D ***NO DATA POINTS*** | | | 126.0, 91.0 | | | |
|  | | |  | | | |

Quantitation Results Report (QT Reviewed)
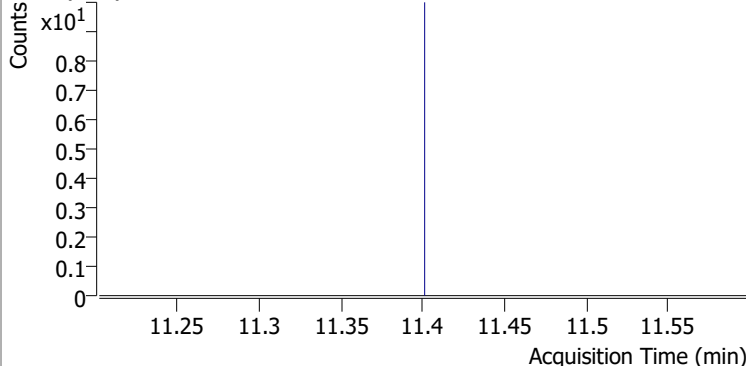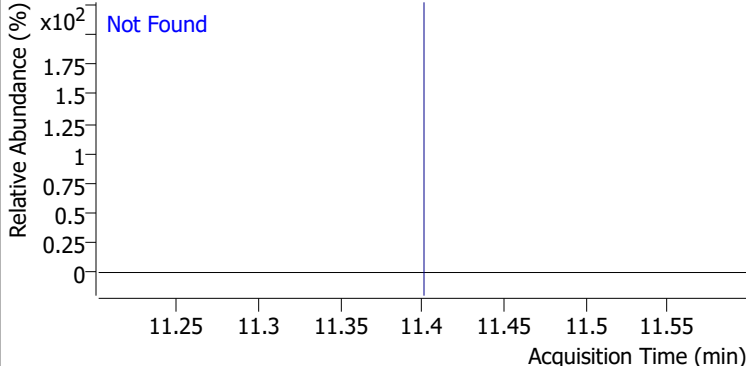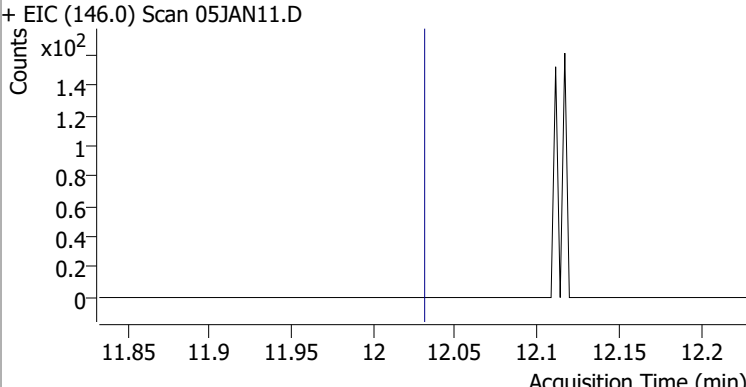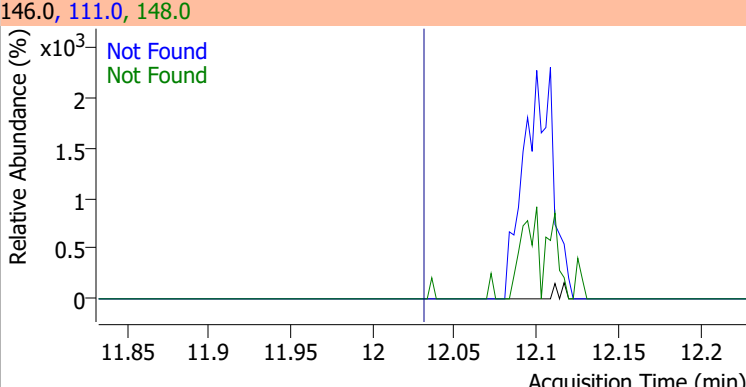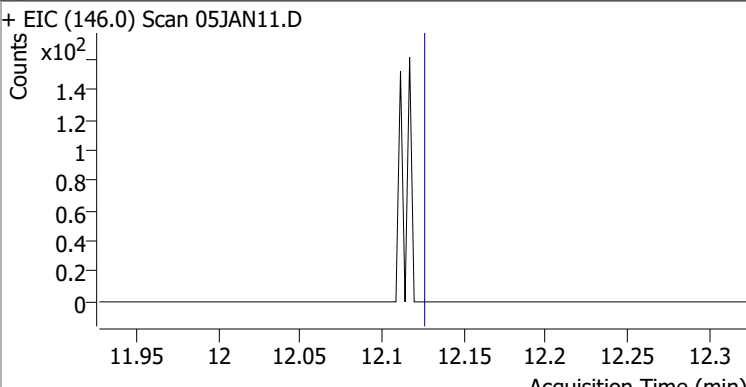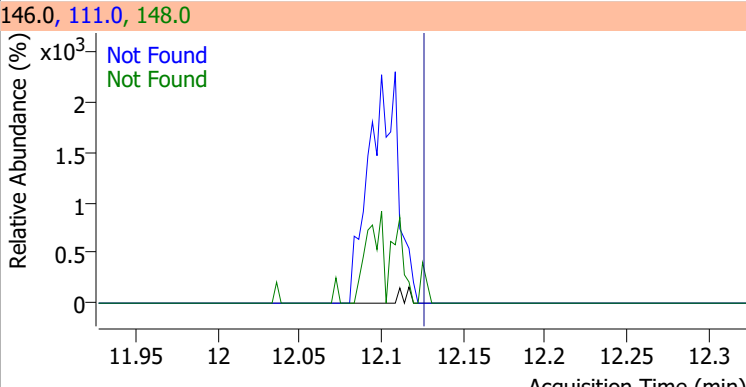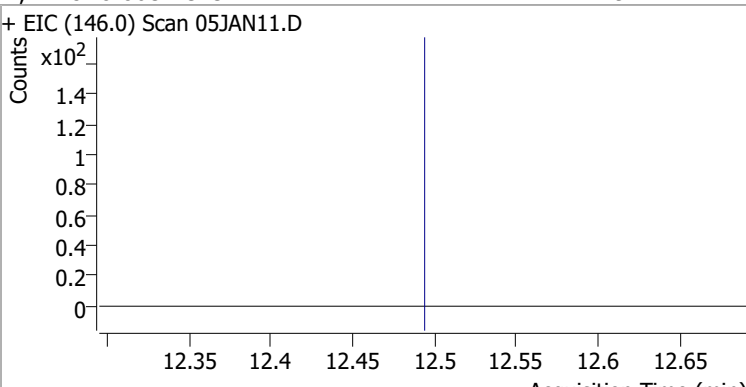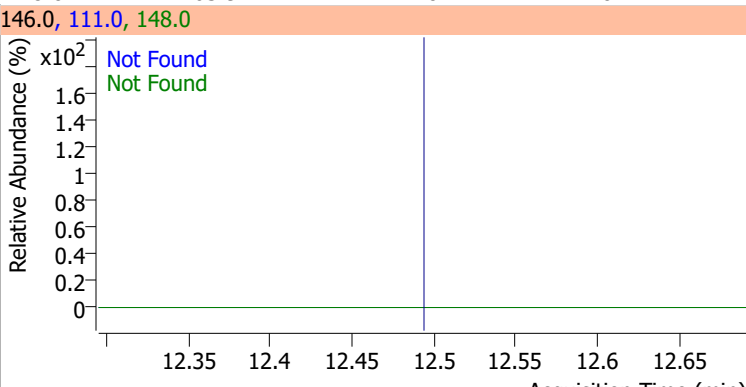
| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--|-------|--------|--|-----------|
| 4-Chlorotoluene | N.D. | 11.40 | 126.0 | 31.7 |
| + EIC (91.0) Scan 05JAN11.D | | | 91.0, 126.0 | |
|  | | |  | |
| 1,3-Dichlorobenzene | N.D. | 12.03 | 148.0 | 63.6 |
| + EIC (146.0) Scan 05JAN11.D | | | 146.0, 111.0, 148.0 | |
|  | | |  | |
| 1,4-Dichlorobenzene | N.D. | 12.13 | 148.0 | 63.1 |
| + EIC (146.0) Scan 05JAN11.D | | | 146.0, 111.0, 148.0 | |
|  | | |  | |
| 1,2-Dichlorobenzene | N.D. | 12.49 | 148.0 | 63.9 |
| + EIC (146.0) Scan 05JAN11.D | | | 146.0, 111.0, 148.0 | |
|  | | |  | |

Quantitation Results Report (QT Reviewed)

| | | | |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File | 05JAN12.D | Operator | MSC |
| Acq. Method | 5975CACQF.M | Acq. Date-Time | 1/5/2022 3:05:50 PM |
| Sample Name | B22010142-002A | Instrument | VOA5975C |
| Vial | 12 | Multiplier | 1.00 |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m | Comment | |
| Tune File | BFB_Atune3.u | Tune Date | 10/11/2021 4:02:00 PM |
| Batch Name | VG010522_8260B.batch.bin | Last Calib Update | 2/28/2022 2:48:47 PM |
| Ref Library | \\MASSHUNTER\Org\Library\NIST129K.I | | |







| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|--------------------|-------|----------|
| Internal Standards | | | | | | |
| M Fluorobenzene | 6.620 | 96.0 | 720040 | 250.0000 | ng | -0.003 |
| M Chlorobenzene-d5 | 9.774 | 82.0 | 283000 | 250.0000 | ng | 0.003 |
| M 1,4-Dichlorobenzene-d4 | 12.100 | 152.0 | 215663 | 250.0000 | ng | 0.000 |
| System Monitoring Compounds | | | | | | |
| S Dibromofluoromethane | 5.845 | 113.0 | 193856 | 285.7755 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 80.0 - 119.0% | | | Recovery = 114.31% | | |
| S 1,2-Dichloroethane-d4 | 6.230 | 67.0 | 84522 | 288.4724 | ng | -0.003 |
| Spiked Amount: 250.000 | Range: 81.0 - 118.0% | | | Recovery = 115.39% | | |
| S Toluene-d8 | 8.322 | 98.0 | 728749 | 267.2217 | ng | 0.003 |
| Spiked Amount: 250.000 | Range: 89.0 - 112.0% | | | Recovery = 106.89% | | |
| S p-Bromofluorobenzene | 10.951 | 95.0 | 214359 | 271.3116 | ng | -0.003 |
| Spiked Amount: 250.000 | Range: 85.0 - 114.0% | | | Recovery = 108.52% | | |
| Target Compounds | | | | | | |
| T Dichlorodifluoromethane | 0.000 | | 0 | N.D. | | |
| T Chloromethane | 1.403 | 50.0 | 1581 | 1.3807 | ng | m |
| T Vinyl chloride | 0.000 | | 0 | N.D. | | |
| T Bromomethane | 0.000 | | 0 | N.D. | | |
| T Chloroethane | 0.000 | | 0 | N.D. | | |
| T Trichlorofluoromethane | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methylene chloride | 3.324 | 49.0 | 2370 | 2.2167 | ng | 93 |
| T trans-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methyl tert-butyl ether (MTBE) | 3.757 | 73.0 | 0 | | ng | md |
| T 1,1-Dichloroethane | 0.000 | | 0 | N.D. | | |
| T 2,2-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T cis-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methyl ethyl ketone | 0.000 | | 0 | N.D. | | |
| T Bromochloromethane | 0.000 | | 0 | N.D. | | |
| T Chloroform | 5.658 | 83.0 | 0 | | ng | md |

Quantitation Results Report (QT Reviewed)

| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|-----------------------------|-------|------|-------|--------|-------|----------|
| T 1,1,1-Trichloroethane | 0.000 | | 0 | N.D. | | |
| T Carbon tetrachloride | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloropropene | 0.000 | | 0 | N.D. | | |
| T Benzene | 6.280 | 78.0 | 411 | 0.1434 | ng m | 87 |
| T 1,2-Dichloroethane | 0.000 | | 0 | N.D. | | |
| T Trichloroethene | 0.000 | | 0 | N.D. | | |
| T 1,2-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T Dibromomethane | 0.000 | | 0 | N.D. | | |
| T Bromodichloromethane | 0.000 | | 0 | N.D. | | |
| T cis-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | |
| T Toluene | 8.380 | 92.0 | 2897 | 1.5726 | ng | 83 |
| T trans-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | |
| T 1,1,2-Trichloroethane | 0.000 | | 0 | N.D. | | |
| T Tetrachloroethene | 0.000 | | 0 | N.D. | | |
| T 1,3-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T Chlorodibromomethane | 0.000 | | 0 | N.D. | | |
| T 1,2-Dibromoethane | 0.000 | | 0 | N.D. | | |
| T Chlorobenzene | 0.000 | | 0 | N.D. | | |
| T 1,1,1,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | |
| T Ethylbenzene | 0.000 | | 0 | N.D. | | |
| T m+p-Xylenes | 0.000 | | 0 | N.D. | | |
| T o-Xylene | 0.000 | | 0 | N.D. | | |
| T Styrene | 0.000 | | 0 | N.D. | | |
| T Bromoform | 0.000 | | 0 | N.D. | | |
| T Bromobenzene | 0.000 | | 0 | N.D. | | |
| T 1,1,2,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | |
| T 1,2,3-Trichloropropane | 0.000 | | 0 | N.D. | | |
| T 2-Chlorotoluene | 0.000 | | 0 | N.D. | | |
| T 4-Chlorotoluene | 0.000 | | 0 | N.D. | | |
| T 1,3-Dichlorobenzene | 0.000 | | 0 | N.D. | | |
| T 1,4-Dichlorobenzene | 0.000 | | 0 | N.D. | | |
| T 1,2-Dichlorobenzene | 0.000 | | 0 | N.D. | | |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)

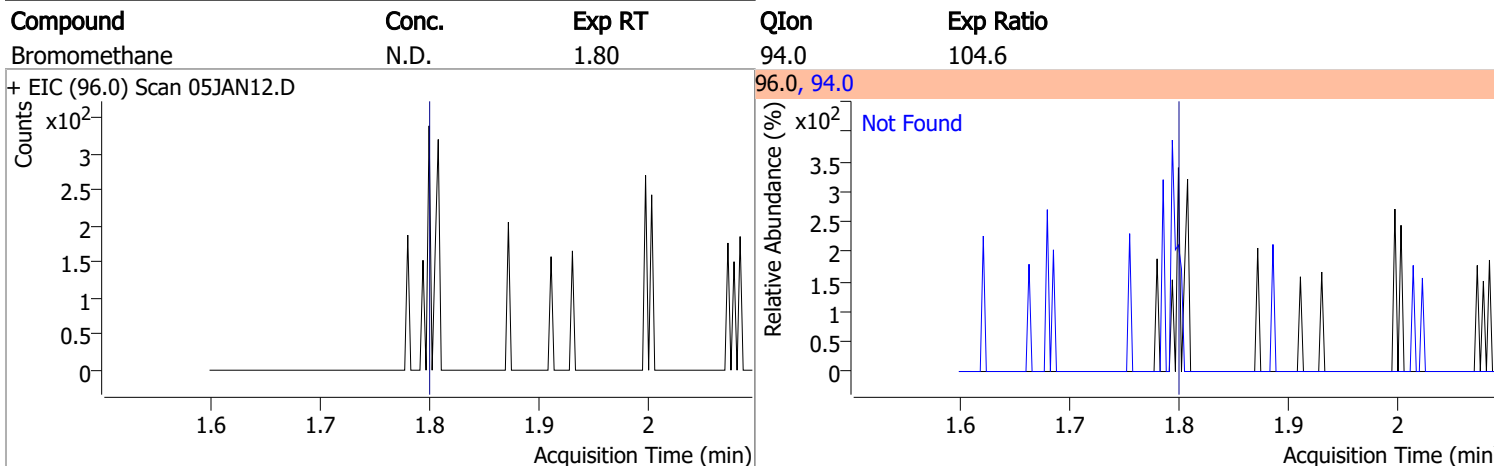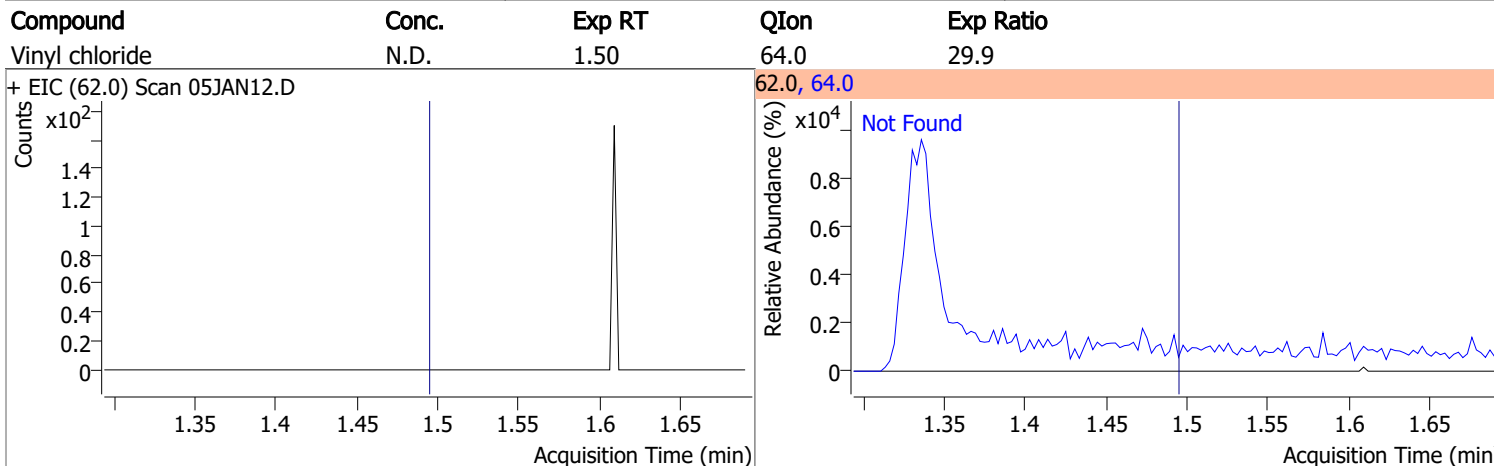


Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------|-------|--------|------|-----------|
| Chloroethane | N.D. | 1.89 | 66.0 | 30.1 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|------------------------|-------|--------|-------|-----------|
| Trichlorofluoromethane | N.D. | 2.14 | 103.0 | 64.2 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethene | N.D. | 2.70 | 61.0 | 180.3 | 63.0 | 56.7 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|--------|------|----------|-------|------|--------|-------|-------|
| Methylene chloride | 2.2167 | 3.32 | -0.01 | 2370 | 84.0 | 60.7 | 36.9 | 96.9 |
| | | | | | 86.0 | 40.1 | 14.3 | 74.3 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,2-Dichloroethene | N.D. | 3.72 | 61.0 | 153.9 | 98.0 | 65.7 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------------------|-------|----|----------|-------|------|--------|-------|-------|
| Methyl tert-butyl ether (MTBE) | | 0 | | 0 | 57.0 | | 0.0 | 54.6 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethane | N.D. | 4.38 | 65.0 | 32.1 | 83.0 | 13.7 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|------|-----------|
| 2,2-Dichloropropane | N.D. | 5.20 | 41.0 | 66.5 | 97.0 | 23.2 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|------------------------|-------|--------|------|-----------|------|-----------|
| cis-1,2-Dichloroethene | N.D. | 5.22 | 61.0 | 167.2 | 98.0 | 67.3 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| Methyl ethyl ketone | N.D. | 5.28 | 72.0 | 21.3 |







| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|
| Bromochloromethane | N.D. | 5.52 | 49.0 | 182.9 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|-------|----|----------|-------|------|--------|-------|-------|
| Chloroform | | 0 | | 0 | 85.0 | | 36.0 | 96.0 |




Quantitation Results Report (QT Reviewed)

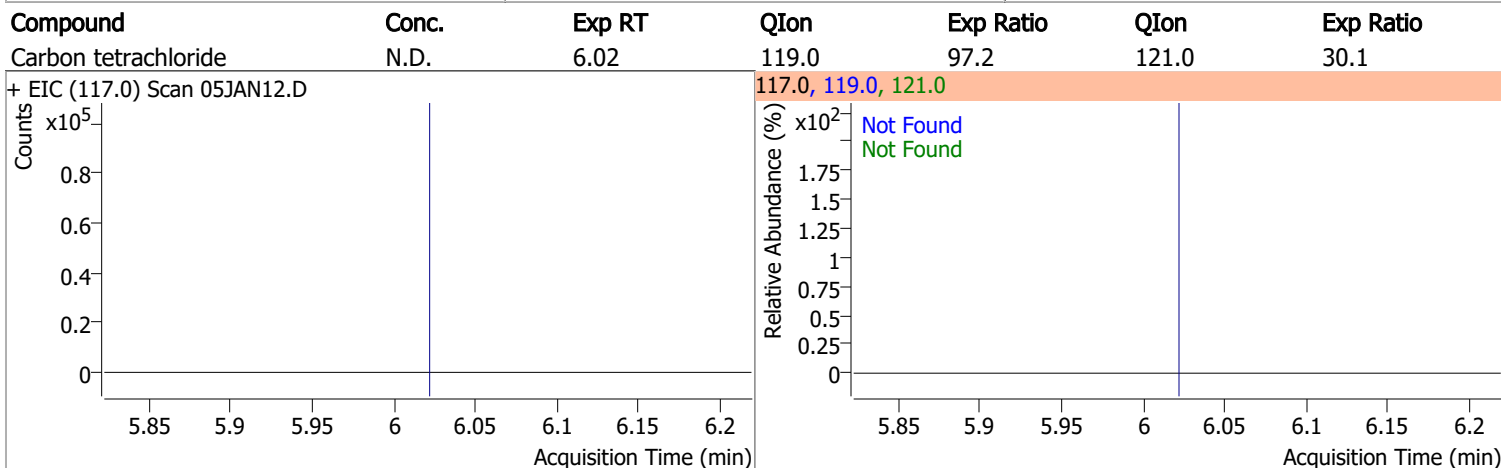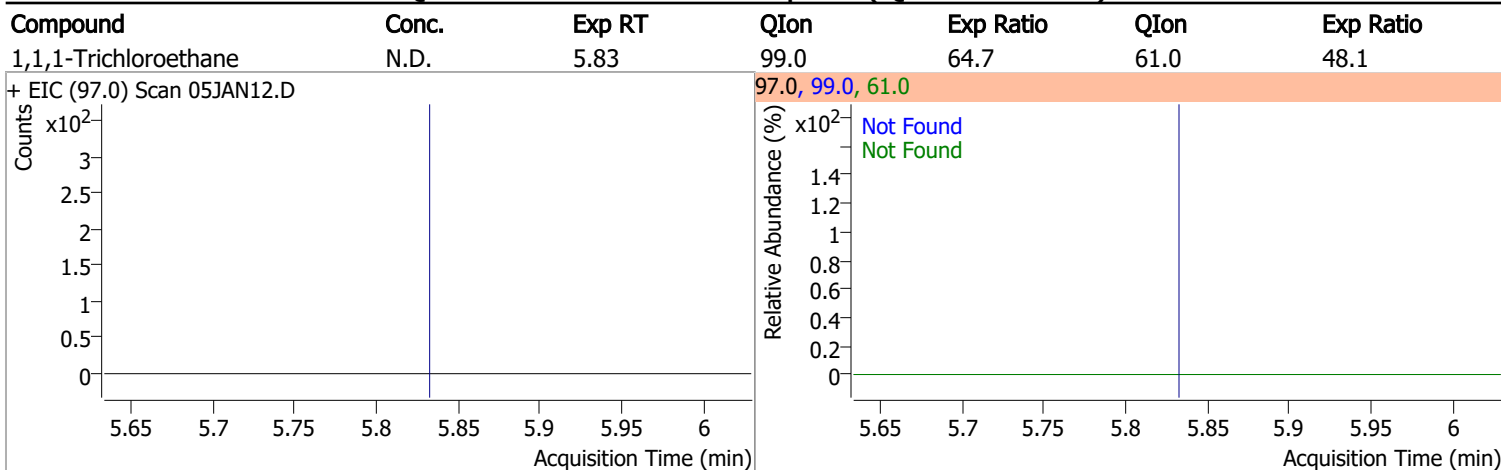


Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 288.4724 | 6.23 | 0.00 | 84522 | 65.0 | 199.3 | 166.5 | 226.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|--------|------|----------|---------|------|--------|-------|-------|
| Benzene | 0.1434 | 6.28 | 0.00 | 411 (m) | 77.0 | 17.0 | 0.0 | 53.5 |











| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,2-Dichloroethane | N.D. | 6.32 | 64.0 | 29.9 | 98.0 | 7.6 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------|-------|--------|-------|-----------|------|-----------|
| Trichloroethene | N.D. | 7.03 | 130.0 | 101.5 | 97.0 | 64.1 |




Quantitation Results Report (QT Reviewed)

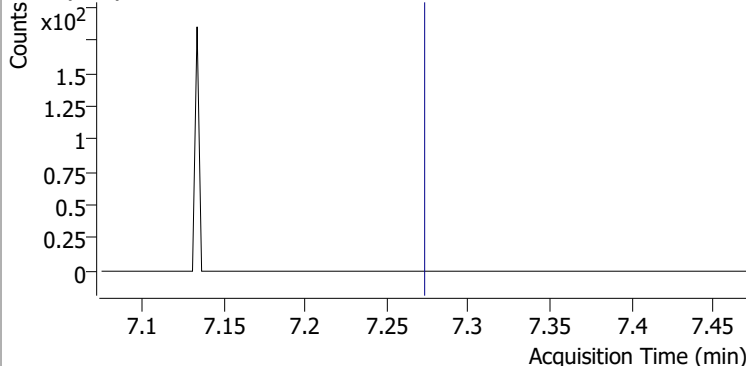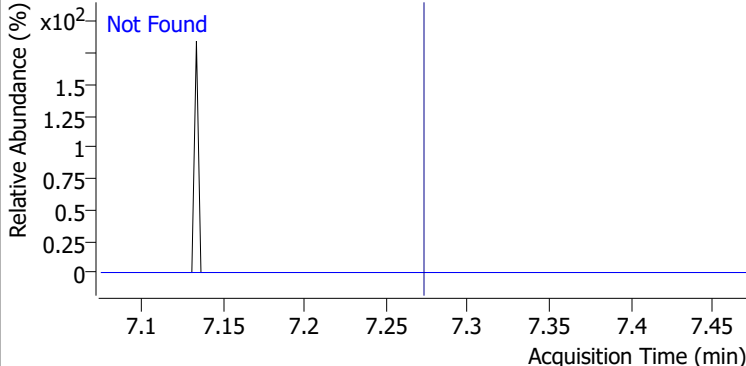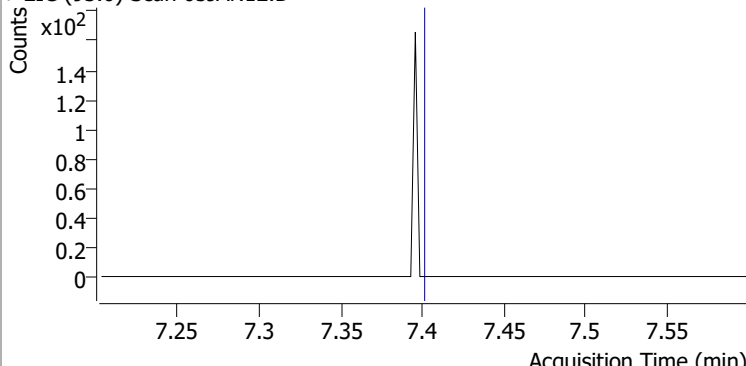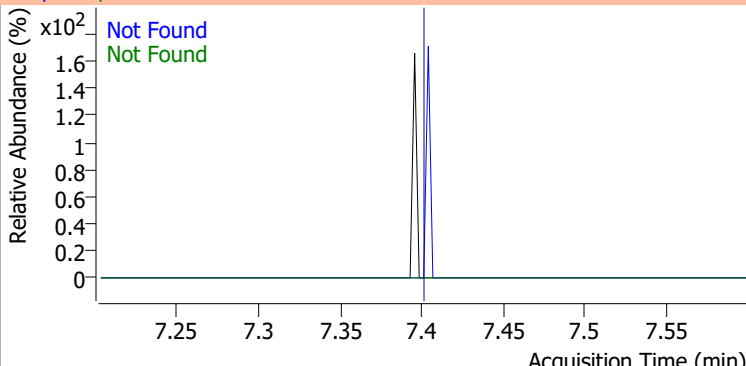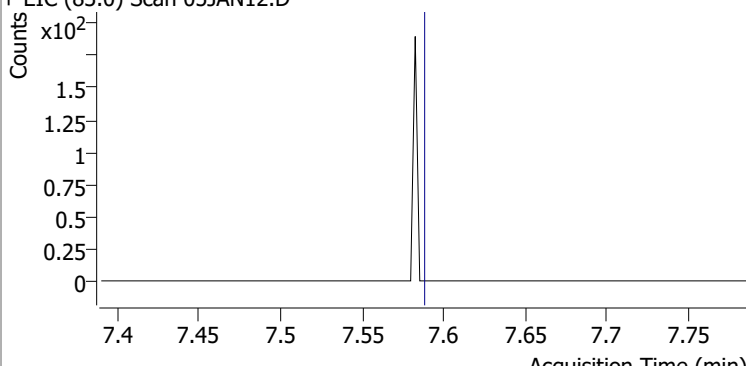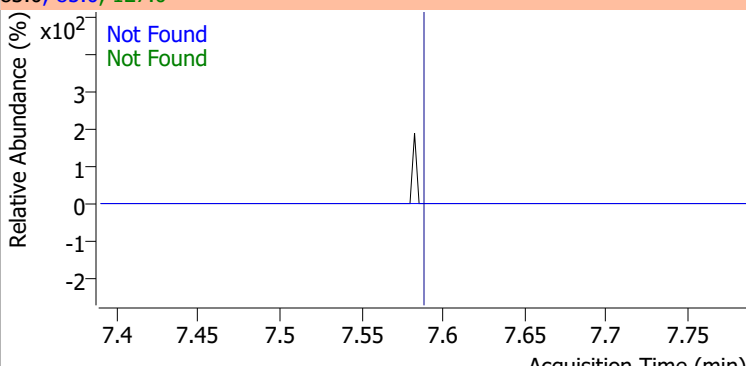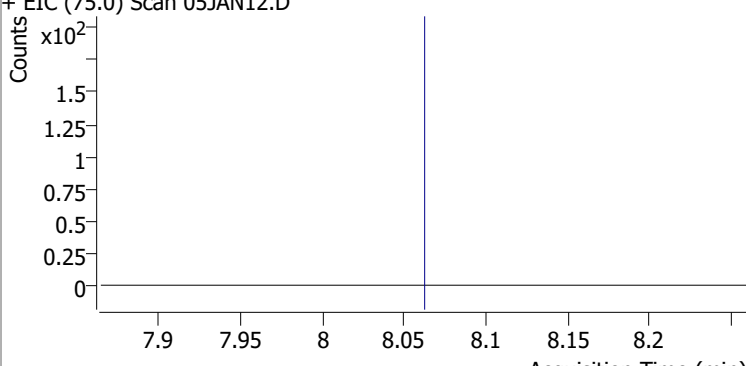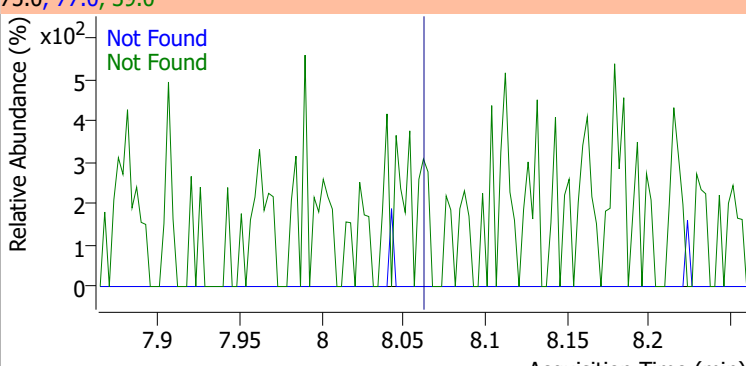
| Compound | Conc. | Exp RT | QIon | Exp Ratio | | |
|--|-------|--------|--|-----------|-------|-----------|
| 1,2-Dichloropropane | N.D. | 7.27 | 76.0 | 38.2 | | |
| + EIC (63.0) Scan 05JAN12.D | | | 63.0, 76.0 | | | |
|  | | |  | | | |
| Dibromomethane | N.D. | 7.40 | 173.5 | 113.7 | QIon | Exp Ratio |
| | | | | | 95.0 | 82.2 |
| + EIC (93.0) Scan 05JAN12.D | | | 93.0, 95.0, 173.5 | | | |
|  | | |  | | | |
| Bromodichloromethane | N.D. | 7.59 | 85.0 | 64.5 | QIon | Exp Ratio |
| | | | | | 127.0 | 9.6 |
| + EIC (83.0) Scan 05JAN12.D | | | 83.0, 85.0, 127.0 | | | |
|  | | |  | | | |
| cis-1,3-Dichloropropene | N.D. | 8.06 | 39.0 | 53.3 | QIon | Exp Ratio |
| | | | | | 77.0 | 31.0 |
| + EIC (75.0) Scan 05JAN12.D | | | 75.0, 77.0, 39.0 | | | |
|  | | |  | | | |

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 267.2217 | 8.32 | 0.00 | 728749 | 100.0 | 63.8 | 34.4 | 94.4 |
| | | | | | 99.0 | 9.5 | 0.0 | 39.6 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|--------|------|----------|-------|------|--------|-------|-------|
| Toluene | 1.5726 | 8.38 | -0.01 | 2897 | 91.0 | 152.4 | 145.8 | 205.8 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,3-Dichloropropene | N.D. | 8.64 | 39.0 | 53.4 | 77.0 | 32.4 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------------|-------|--------|------|-----------|------|-----------|
| 1,1,2-Trichloroethane | N.D. | 8.82 | 97.0 | 114.6 | 85.0 | 67.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-------------------|-------|--------|-------|-----------|-------|-----------|
| Tetrachloroethene | N.D. | 8.94 | 165.8 | 128.6 | 129.0 | 91.5 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| 1,3-Dichloropropane | N.D. | 8.98 | 78.0 | 32.9 |











| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------------------|-------|--------|-------|-----------|
| Chlorodibromomethane | N.D. | 9.21 | 127.0 | 78.0 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|-------------------|-------|--------|-------|-----------|
| 1,2-Dibromoethane | N.D. | 9.31 | 109.0 | 94.5 |




Quantitation Results Report (QT Reviewed)

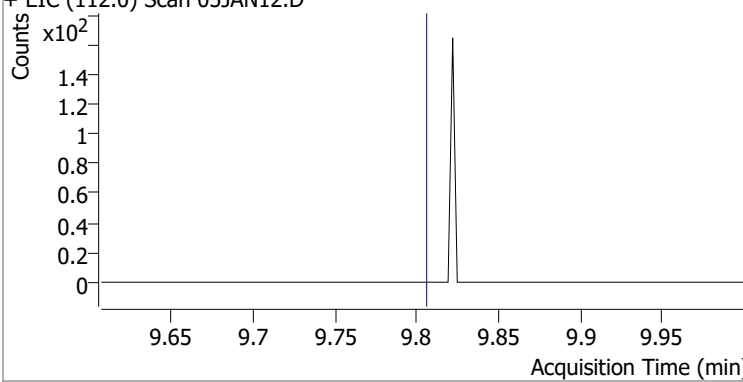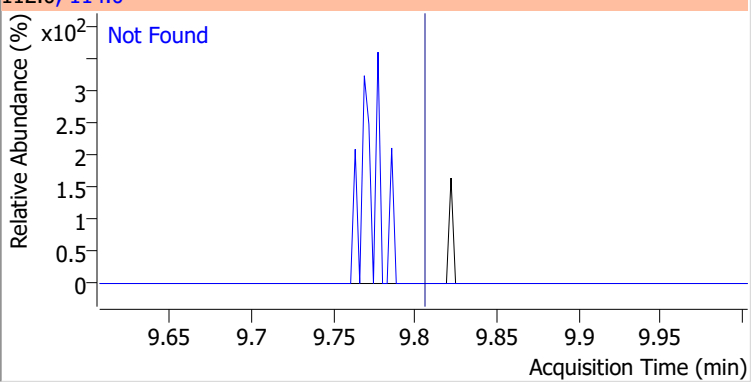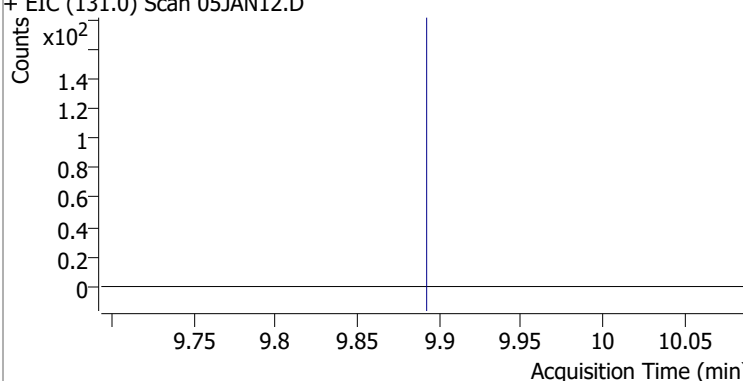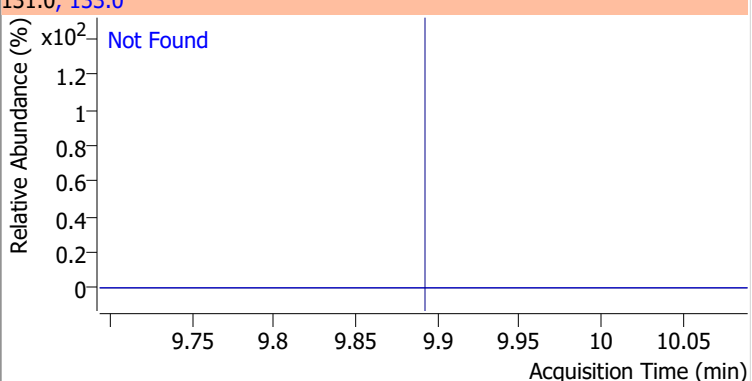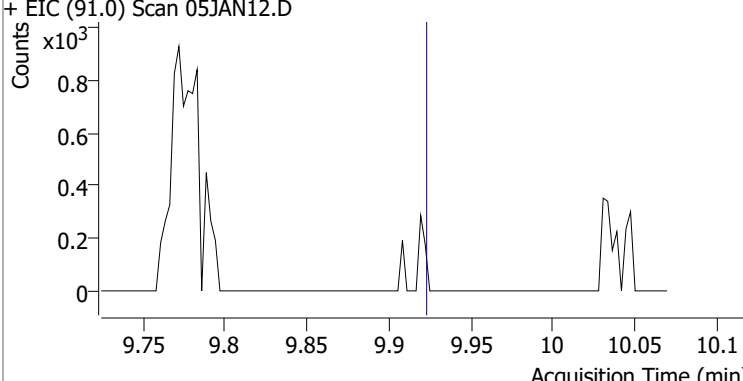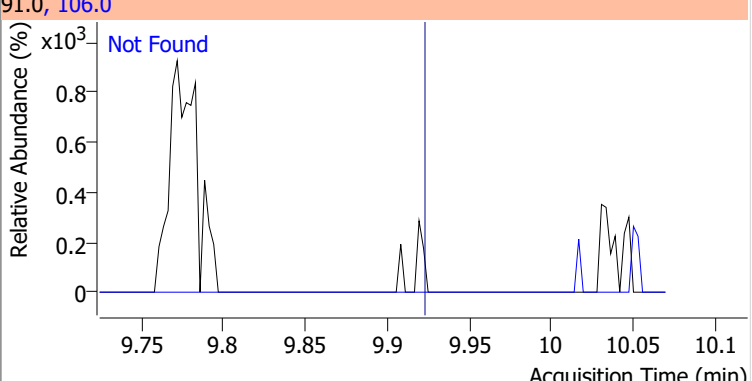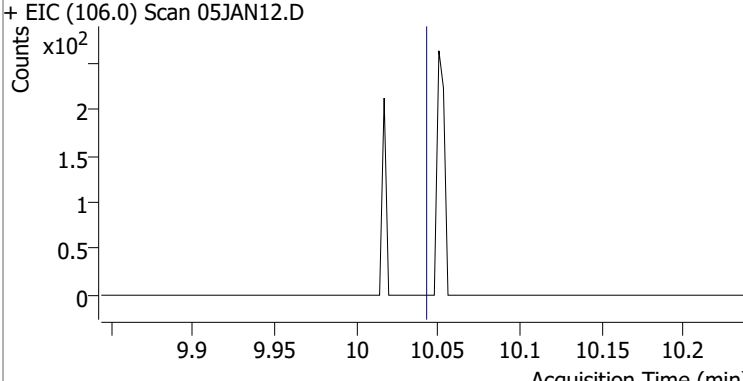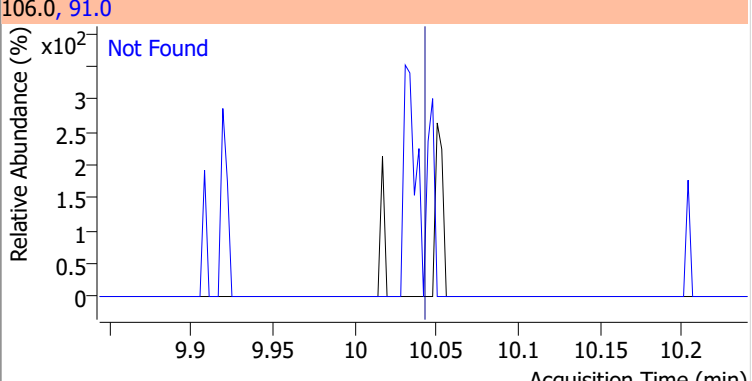
| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--|-------|--------|--|-----------|
| Chlorobenzene | N.D. | 9.80 | 114.0 | 32.1 |
| + EIC (112.0) Scan 05JAN12.D | | | 112.0, 114.0 | |
|  | | |  | |
| 1,1,1,2-Tetrachloroethane | N.D. | 9.89 | 133.0 | 98.6 |
| + EIC (131.0) Scan 05JAN12.D | | | 131.0, 133.0 | |
|  | | |  | |
| Ethylbenzene | N.D. | 9.92 | 106.0 | 31.1 |
| + EIC (91.0) Scan 05JAN12.D | | | 91.0, 106.0 | |
|  | | |  | |
| m+p-Xylenes | N.D. | 10.04 | 91.0 | 201.4 |
| + EIC (106.0) Scan 05JAN12.D | | | 106.0, 91.0 | |
|  | | |  | |

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------|-------|--------|------|-----------|
| o-Xylene | N.D. | 10.43 | 91.0 | 213.1 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------|-------|--------|------|-----------|
| Styrene | N.D. | 10.45 | 78.0 | 49.6 |











| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------|-------|--------|-------|-----------|-------|-----------|
| Bromoform | N.D. | 10.63 | 170.5 | 52.1 | 174.5 | 50.1 |











| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 271.3116 | 10.95 | 0.00 | 214359 | 174.0 | 93.9 | 61.7 | 121.7 |
| | | | | | 176.0 | 90.5 | 60.6 | 120.6 |



Quantitation Results Report (QT Reviewed)

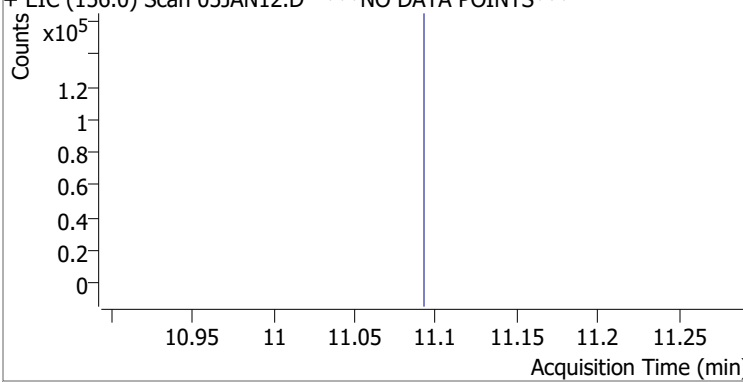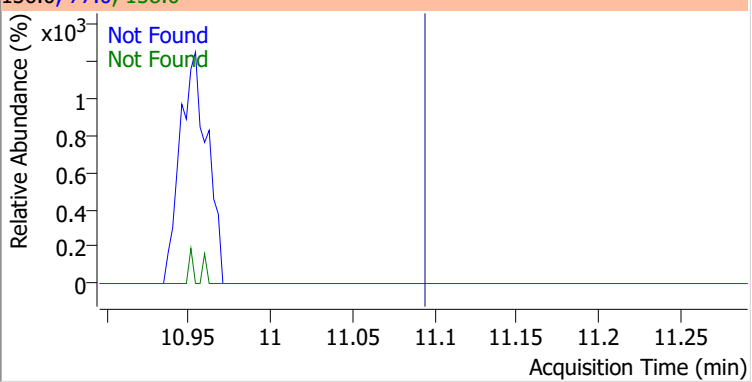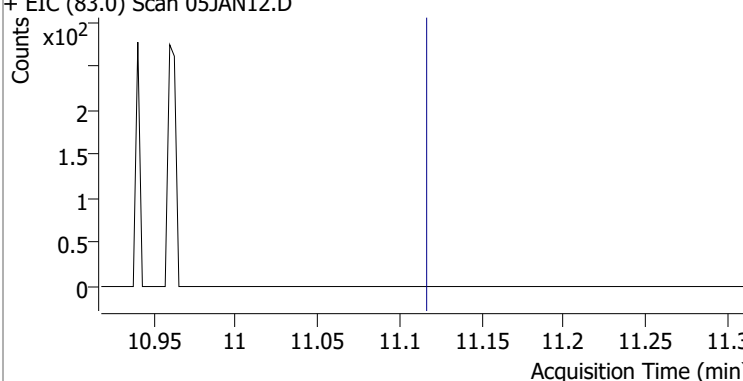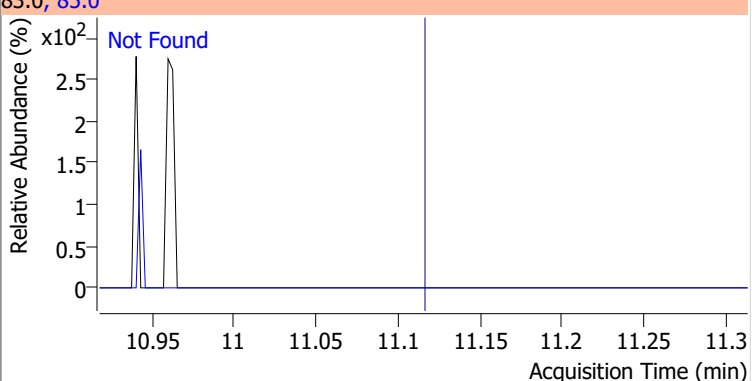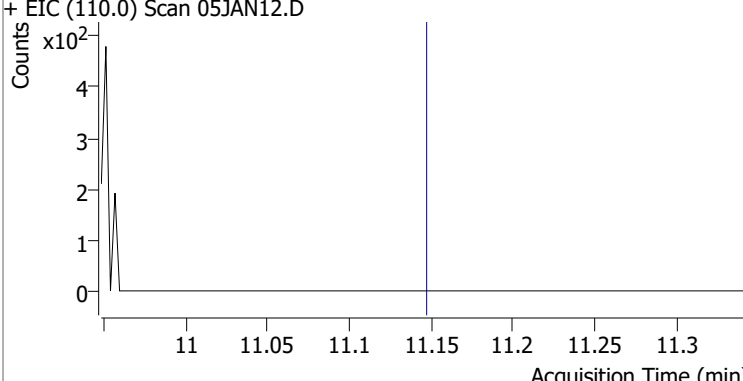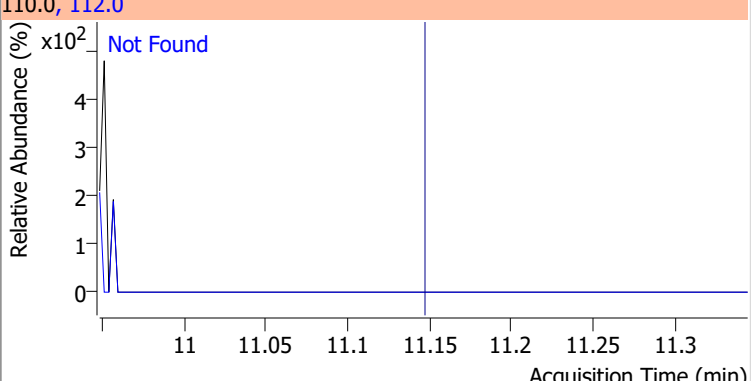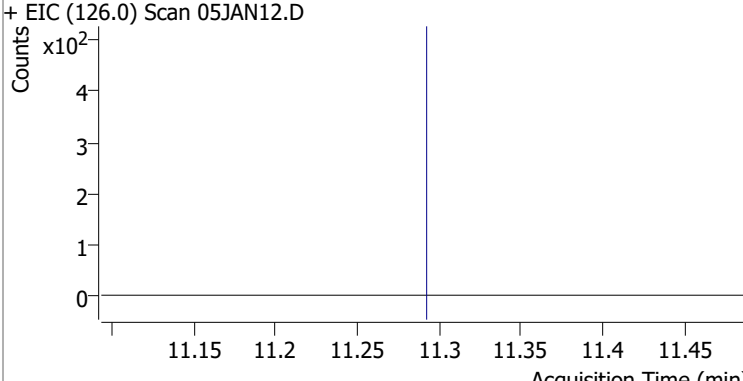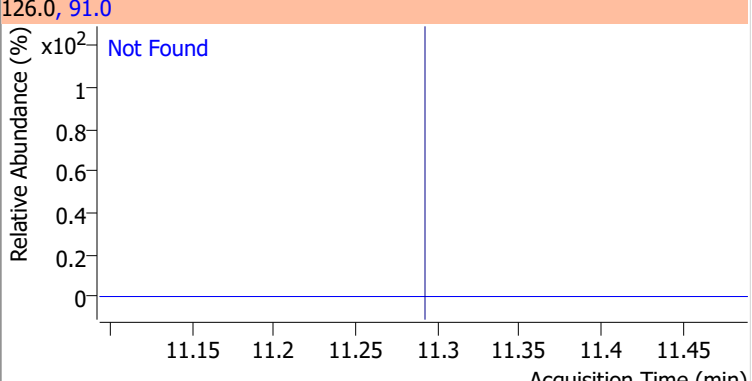
| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--|-------|--------|--|-----------|-------|-----------|
| Bromobenzene | N.D. | 11.09 | 77.0 | 145.7 | 158.0 | 96.5 |
| + EIC (156.0) Scan 05JAN12.D ***NO DATA POINTS*** | | | 156.0, 77.0, 158.0 | | | |
|  | | |  | | | |
| 1,1,2,2-Tetrachloroethane | N.D. | 11.12 | 85.0 | 66.2 | | |
| + EIC (83.0) Scan 05JAN12.D | | | 83.0, 85.0 | | | |
|  | | |  | | | |
| 1,2,3-Trichloropropane | N.D. | 11.15 | 112.0 | 63.5 | | |
| + EIC (110.0) Scan 05JAN12.D | | | 110.0, 112.0 | | | |
|  | | |  | | | |
| 2-Chlorotoluene | N.D. | 11.29 | 91.0 | 282.3 | | |
| + EIC (126.0) Scan 05JAN12.D | | | 126.0, 91.0 | | | |
|  | | |  | | | |

Quantitation Results Report (QT Reviewed)
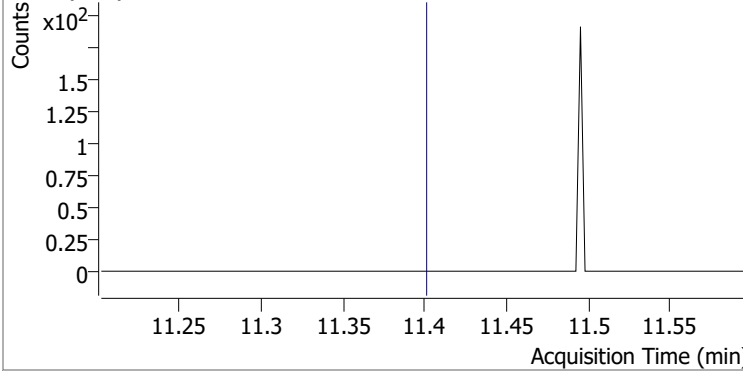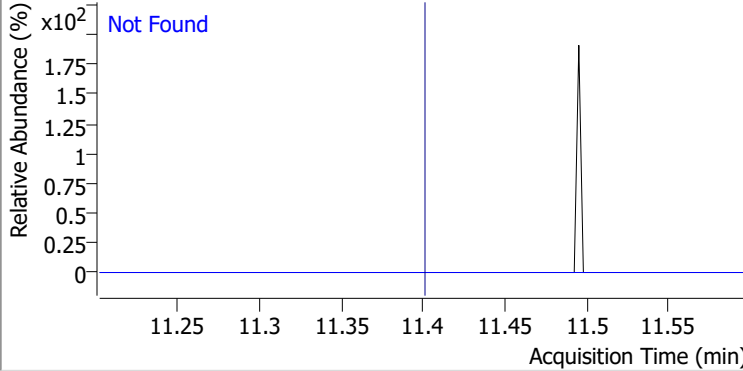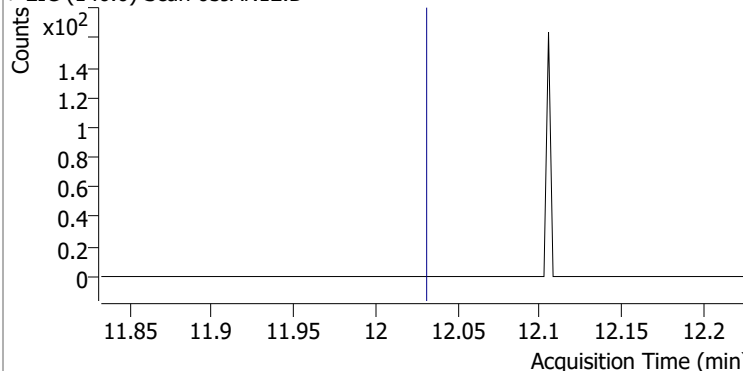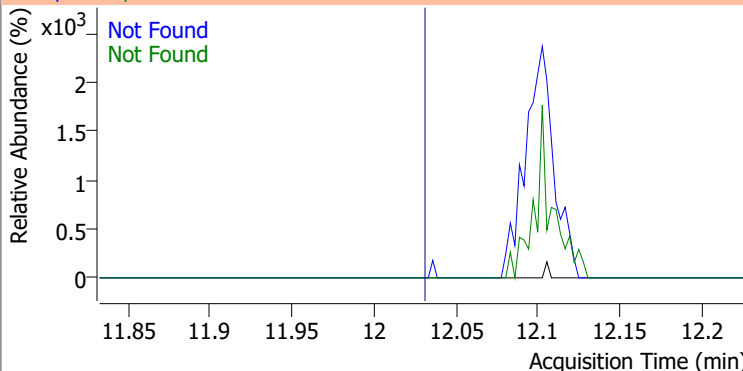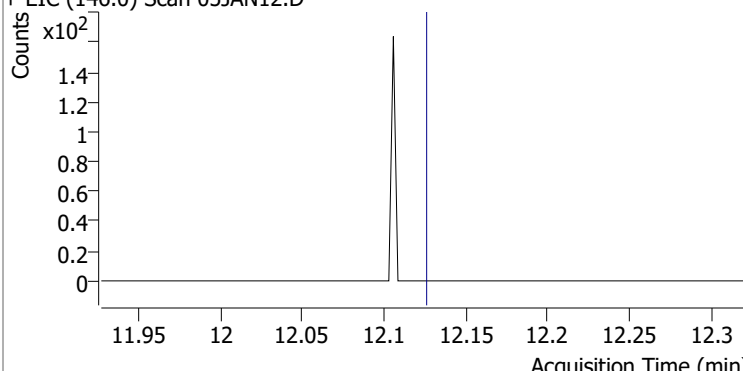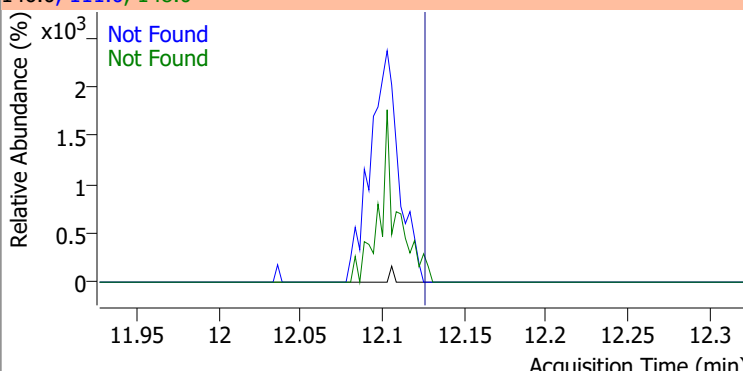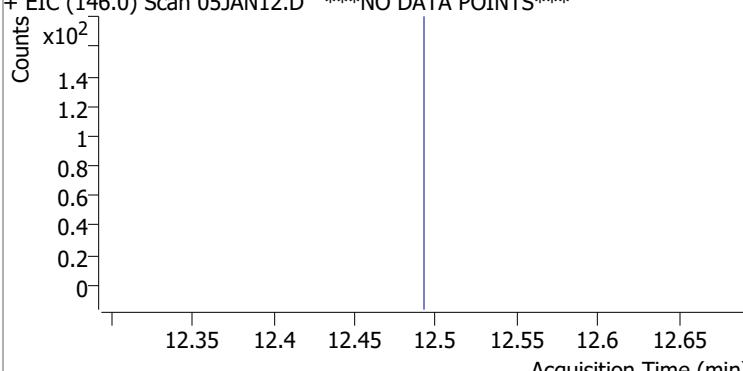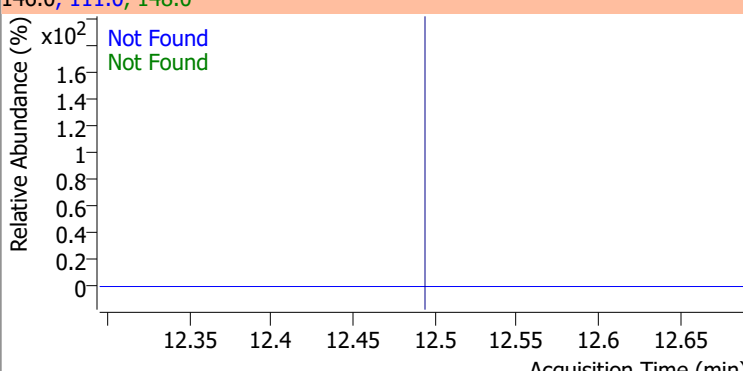
| Compound | Conc. | Exp RT | QIon | Exp Ratio | | |
|--|-------|--------|--|-----------|------|-----------|
| 4-Chlorotoluene | N.D. | 11.40 | 126.0 | 31.7 | | |
| + EIC (91.0) Scan 05JAN12.D | | | 91.0, 126.0 | | | |
|  | | |  | | | |
| 1,3-Dichlorobenzene | N.D. | 12.03 | 148.0 | 63.6 | QIon | Exp Ratio |
| + EIC (146.0) Scan 05JAN12.D | | | 146.0, 111.0, 148.0 | | | |
|  | | |  | | | |
| 1,4-Dichlorobenzene | N.D. | 12.13 | 148.0 | 63.1 | QIon | Exp Ratio |
| + EIC (146.0) Scan 05JAN12.D | | | 146.0, 111.0, 148.0 | | | |
|  | | |  | | | |
| 1,2-Dichlorobenzene | N.D. | 12.49 | 148.0 | 63.9 | QIon | Exp Ratio |
| + EIC (146.0) Scan 05JAN12.D ***NO DATA POINTS*** | | | 146.0, 111.0, 148.0 | | | |
|  | | |  | | | |

Quantitation Results Report (QT Reviewed)

| | | | |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File | 05JAN13.D | Operator | MSC |
| Acq. Method | 5975CACQF.M | Acq. Date-Time | 1/5/2022 3:33:12 PM |
| Sample Name | B22010143-002A | Instrument | VOA5975C |
| Vial | 13 | Multiplier | 1.00 |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m | Comment | |
| Tune File | BFB_Atune3.u | Tune Date | 10/11/2021 4:02:00 PM |
| Batch Name | VG010522_8260B.batch.bin | Last Calib Update | 2/28/2022 2:48:47 PM |
| Ref Library | \\MASSHUNTER\Org\Library\NIST129K.I | | |







| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|--------------------|-------|----------|
| Internal Standards | | | | | | |
| M Fluorobenzene | 6.620 | 96.0 | 730262 | 250.0000 | ng | -0.003 |
| M Chlorobenzene-d5 | 9.774 | 82.0 | 285143 | 250.0000 | ng | 0.003 |
| M 1,4-Dichlorobenzene-d4 | 12.103 | 152.0 | 216732 | 250.0000 | ng | 0.003 |
| System Monitoring Compounds | | | | | | |
| S Dibromofluoromethane | 5.848 | 113.0 | 191770 | 278.7432 | ng | 0.003 |
| Spiked Amount: 250.000 | Range: 80.0 - 119.0% | | | Recovery = 111.50% | | |
| S 1,2-Dichloroethane-d4 | 6.233 | 67.0 | 83556 | 281.1836 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 81.0 - 118.0% | | | Recovery = 112.47% | | |
| S Toluene-d8 | 8.319 | 98.0 | 733310 | 266.8733 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 89.0 - 112.0% | | | Recovery = 106.75% | | |
| S p-Bromofluorobenzene | 10.951 | 95.0 | 210682 | 265.3424 | ng | -0.003 |
| Spiked Amount: 250.000 | Range: 85.0 - 114.0% | | | Recovery = 106.14% | | |
| Target Compounds | | | | | | |
| T Dichlorodifluoromethane | 0.000 | | 0 | N.D. | | |
| T Chloromethane | 1.400 | 50.0 | 955 | 0.8223 | ng | m 81 |
| T Vinyl chloride | 0.000 | | 0 | N.D. | | |
| T Bromomethane | 0.000 | | 0 | N.D. | | |
| T Chloroethane | 0.000 | | 0 | N.D. | | |
| T Trichlorofluoromethane | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methylene chloride | 3.324 | 49.0 | 1841 | 1.6977 | ng | m 87 |
| T trans-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methyl tert-butyl ether (MTBE) | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloroethane | 0.000 | | 0 | N.D. | | |
| T 2,2-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T cis-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methyl ethyl ketone | 0.000 | | 0 | N.D. | | |
| T Bromochloromethane | 0.000 | | 0 | N.D. | | |
| T Chloroform | 0.000 | | 0 | N.D. | | |

Quantitation Results Report (QT Reviewed)




| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|-----------------------------|-------|------|-------|--------|-------|----------|
| T 1,1,1-Trichloroethane | 0.000 | | 0 | N.D. | | |
| T Carbon tetrachloride | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloropropene | 0.000 | | 0 | N.D. | | |
| T Benzene | 0.000 | | 0 | N.D. | | |
| T 1,2-Dichloroethane | 0.000 | | 0 | N.D. | | |
| T Trichloroethene | 0.000 | | 0 | N.D. | | |
| T 1,2-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T Dibromomethane | 0.000 | | 0 | N.D. | | |
| T Bromodichloromethane | 0.000 | | 0 | N.D. | | |
| T cis-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | |
| T Toluene | 8.383 | 92.0 | 3027 | 1.6308 | ng | 84 |
| T trans-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | |
| T 1,1,2-Trichloroethane | 0.000 | | 0 | N.D. | | |
| T Tetrachloroethene | 0.000 | | 0 | N.D. | | |
| T 1,3-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T Chlorodibromomethane | 0.000 | | 0 | N.D. | | |
| T 1,2-Dibromoethane | 0.000 | | 0 | N.D. | | |
| T Chlorobenzene | 0.000 | | 0 | N.D. | | |
| T 1,1,1,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | |
| T Ethylbenzene | 0.000 | | 0 | N.D. | | |
| T m+p-Xylenes | 0.000 | | 0 | N.D. | | |
| T o-Xylene | 0.000 | | 0 | N.D. | | |
| T Styrene | 0.000 | | 0 | N.D. | | |
| T Bromoform | 0.000 | | 0 | N.D. | | |
| T Bromobenzene | 0.000 | | 0 | N.D. | | |
| T 1,1,2,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | |
| T 1,2,3-Trichloropropane | 0.000 | | 0 | N.D. | | |
| T 2-Chlorotoluene | 0.000 | | 0 | N.D. | | |
| T 4-Chlorotoluene | 0.000 | | 0 | N.D. | | |
| T 1,3-Dichlorobenzene | 0.000 | | 0 | N.D. | | |
| T 1,4-Dichlorobenzene | 0.000 | | 0 | N.D. | | |
| T 1,2-Dichlorobenzene | 0.000 | | 0 | N.D. | | |

(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak


Quantitation Results Report (QT Reviewed)

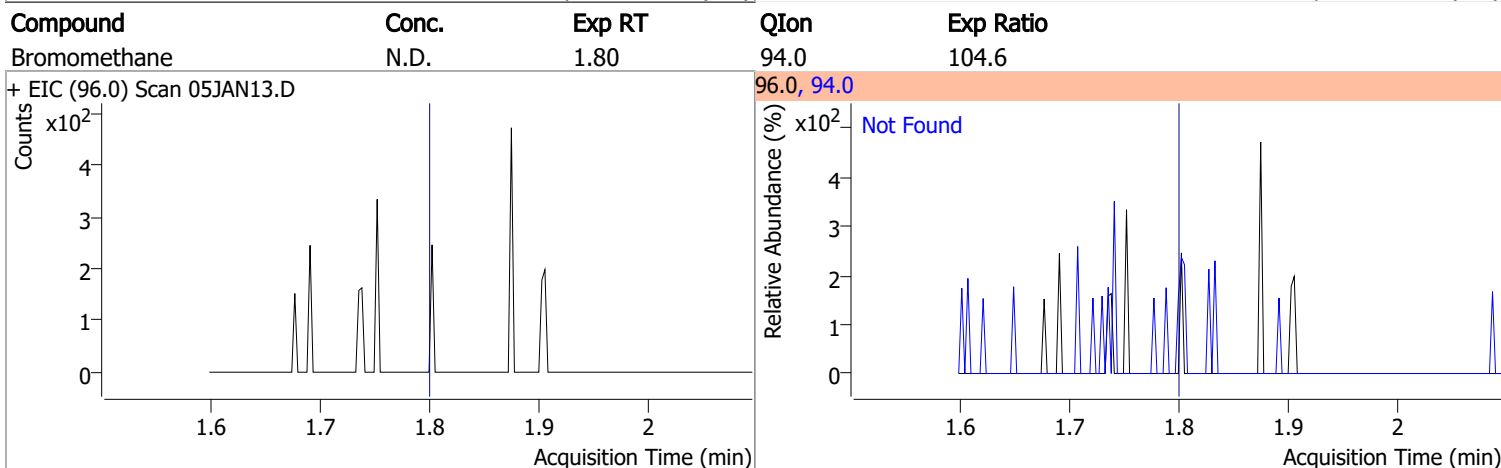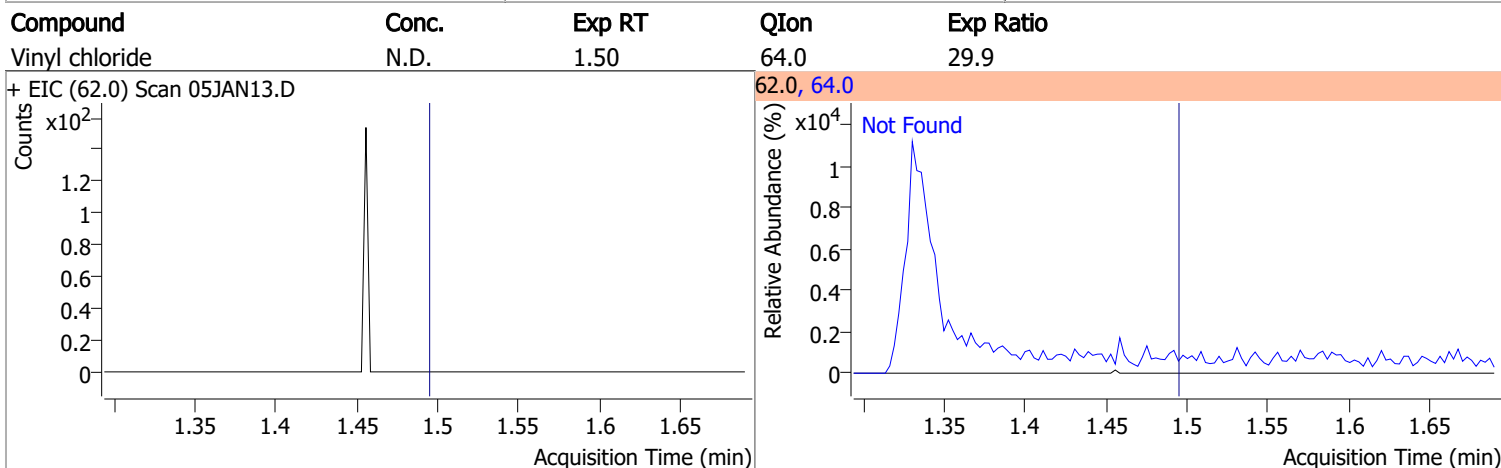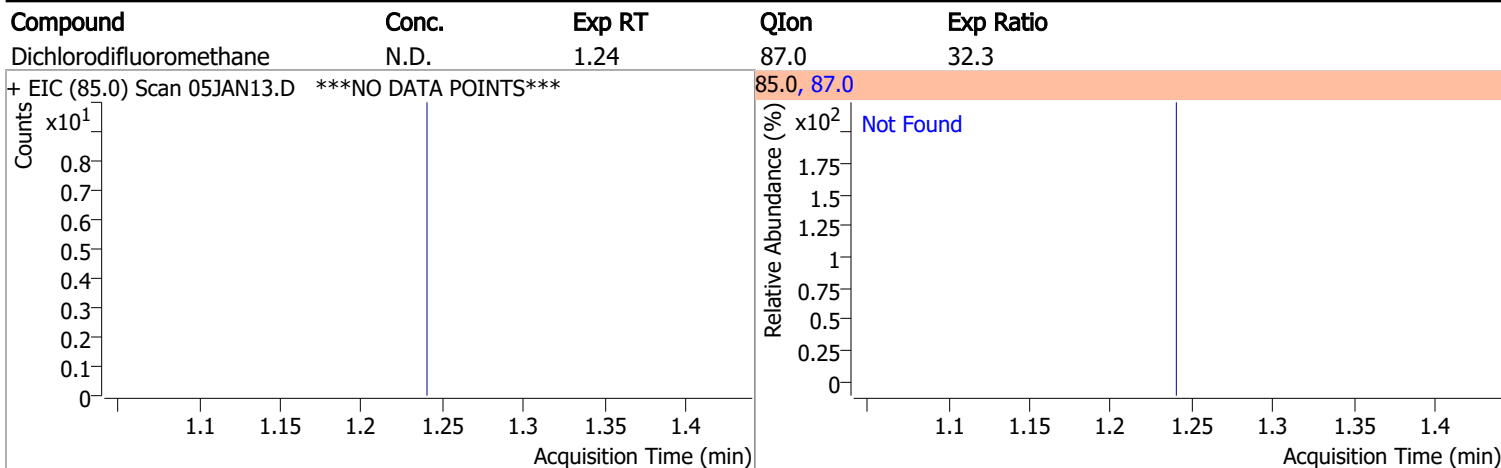

Quantitation Results Report (QT Reviewed)

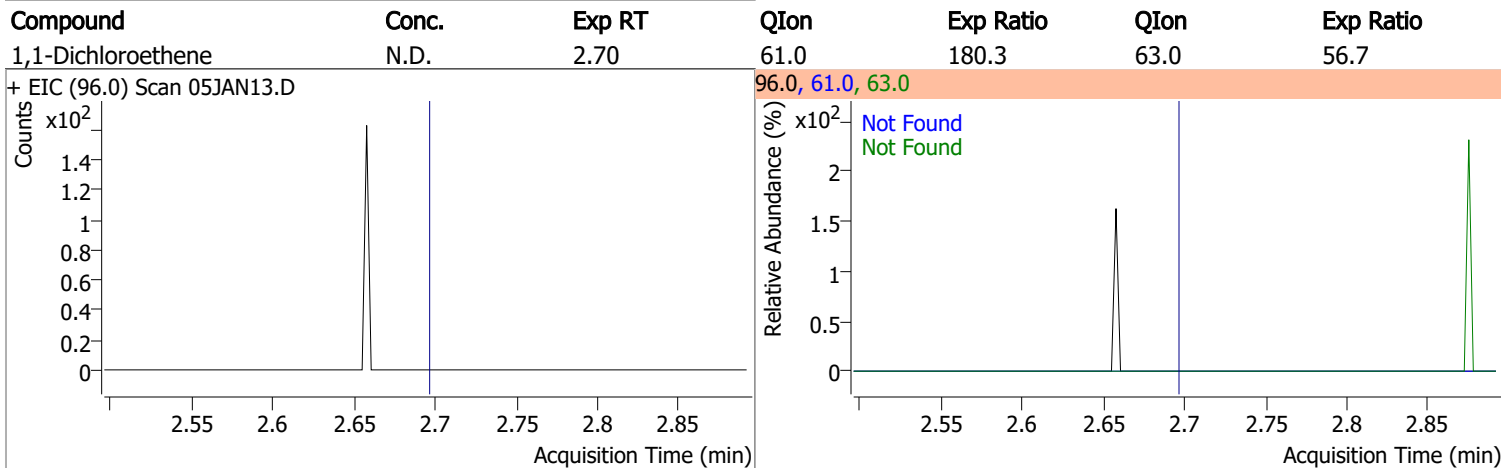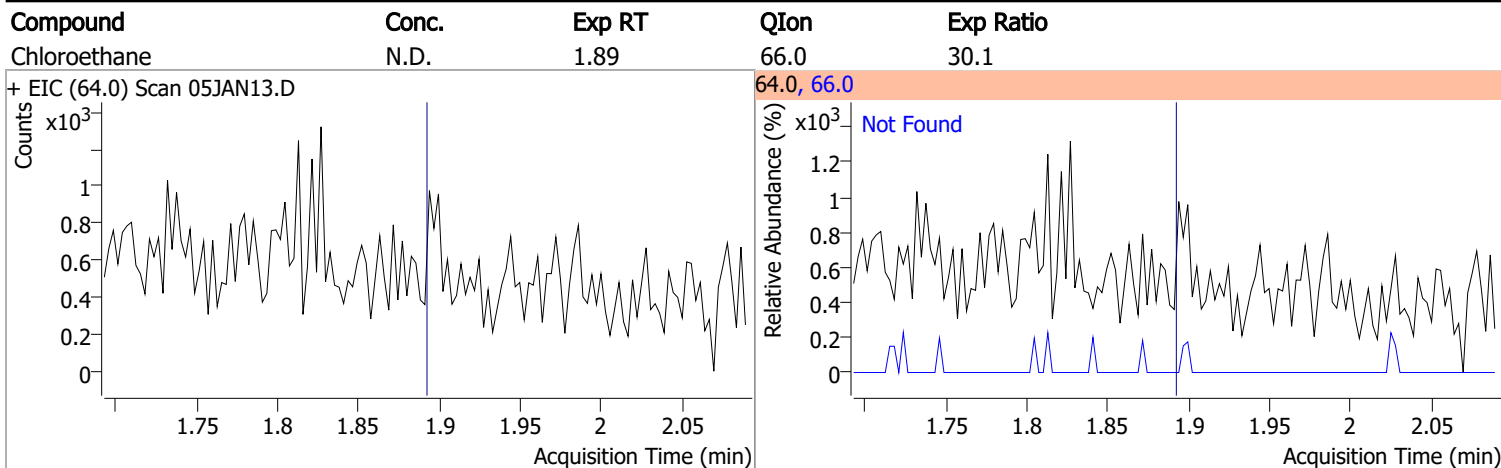


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|--------|------|----------|----------|------|--------|-------|-------|
| Methylene chloride | 1.6977 | 3.32 | -0.01 | 1841 (m) | 84.0 | 80.0 | 36.9 | 96.9 |
| | | | | | 86.0 | 39.5 | 14.3 | 74.3 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,2-Dichloroethene | N.D. | 3.72 | 61.0 | 153.9 | 98.0 | 65.7 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------------------|-------|--------|------|-----------|
| Methyl tert-butyl ether (MTBE) | N.D. | 3.75 | 57.0 | 24.6 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethane | N.D. | 4.38 | 65.0 | 32.1 | 83.0 | 13.7 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|------|-----------|
| 2,2-Dichloropropane | N.D. | 5.20 | 41.0 | 66.5 | 97.0 | 23.2 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|------------------------|-------|--------|------|-----------|------|-----------|
| cis-1,2-Dichloroethene | N.D. | 5.22 | 61.0 | 167.2 | 98.0 | 67.3 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| Methyl ethyl ketone | N.D. | 5.28 | 72.0 | 21.3 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|
| Bromochloromethane | N.D. | 5.52 | 49.0 | 182.9 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|------------|-------|--------|------|-----------|
| Chloroform | N.D. | 5.65 | 85.0 | 66.0 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------------|-------|--------|------|-----------|------|-----------|
| 1,1,1-Trichloroethane | N.D. | 5.83 | 99.0 | 64.7 | 61.0 | 48.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Dibromofluoromethane | 278.7432 | 5.85 | 0.00 | 191770 | 191.5 | 22.1 | 0.0 | 53.1 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|----------------------|-------|--------|-------|-----------|-------|-----------|
| Carbon tetrachloride | N.D. | 6.02 | 119.0 | 97.2 | 121.0 | 30.1 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|-------|-----------|------|-----------|
| 1,1-Dichloropropene | N.D. | 6.04 | 110.0 | 35.9 | 77.0 | 30.1 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 281.1836 | 6.23 | 0.00 | 83556 | 65.0 | 202.0 | 166.5 | 226.5 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------|-------|--------|------|-----------|
| Benzene | N.D. | 6.28 | 77.0 | 23.5 |







| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,2-Dichloroethane | N.D. | 6.32 | 64.0 | 29.9 | 98.0 | 7.6 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------|-------|--------|-------|-----------|------|-----------|
| Trichloroethene | N.D. | 7.03 | 130.0 | 101.5 | 97.0 | 64.1 |




Quantitation Results Report (QT Reviewed)

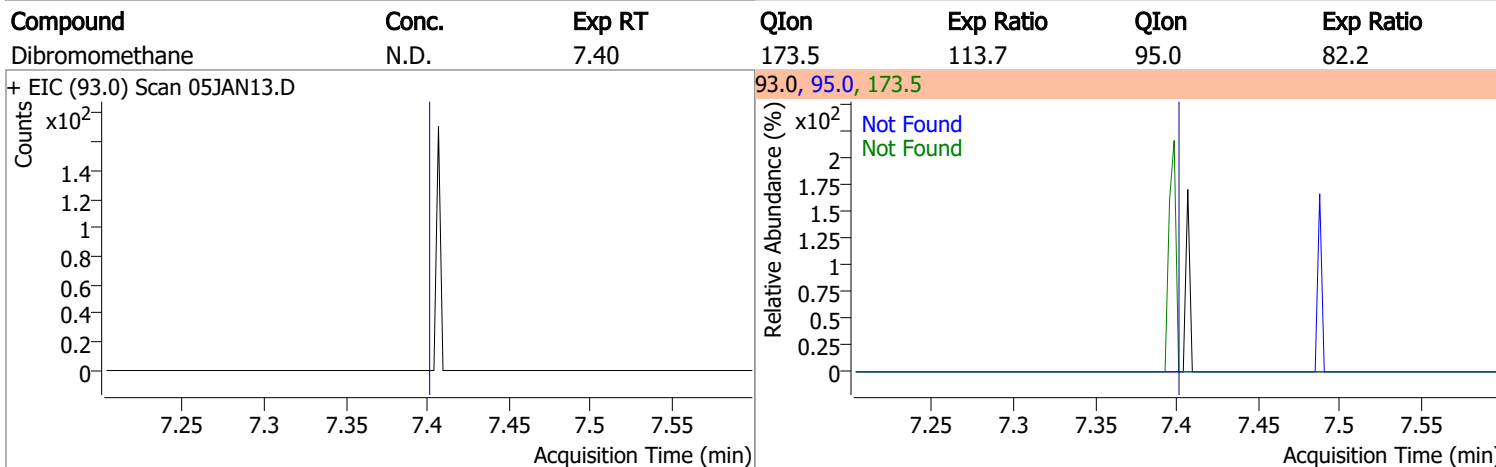


Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 266.8733 | 8.32 | 0.00 | 733310 | 100.0 | 63.7 | 34.4 | 94.4 |
| | | | | | 99.0 | 9.6 | 0.0 | 39.6 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|--------|------|----------|-------|------|--------|-------|-------|
| Toluene | 1.6308 | 8.38 | -0.01 | 3027 | 91.0 | 153.8 | 145.8 | 205.8 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,3-Dichloropropene | N.D. | 8.64 | 39.0 | 53.4 | 77.0 | 32.4 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------------|-------|--------|------|-----------|------|-----------|
| 1,1,2-Trichloroethane | N.D. | 8.82 | 97.0 | 114.6 | 85.0 | 67.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-------------------|-------|--------|-------|-----------|-------|-----------|
| Tetrachloroethene | N.D. | 8.94 | 165.8 | 128.6 | 129.0 | 91.5 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| 1,3-Dichloropropane | N.D. | 8.98 | 78.0 | 32.9 |











| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------------------|-------|--------|-------|-----------|
| Chlorodibromomethane | N.D. | 9.21 | 127.0 | 78.0 |






| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|-------------------|-------|--------|-------|-----------|
| 1,2-Dibromoethane | N.D. | 9.31 | 109.0 | 94.5 |




Quantitation Results Report (QT Reviewed)
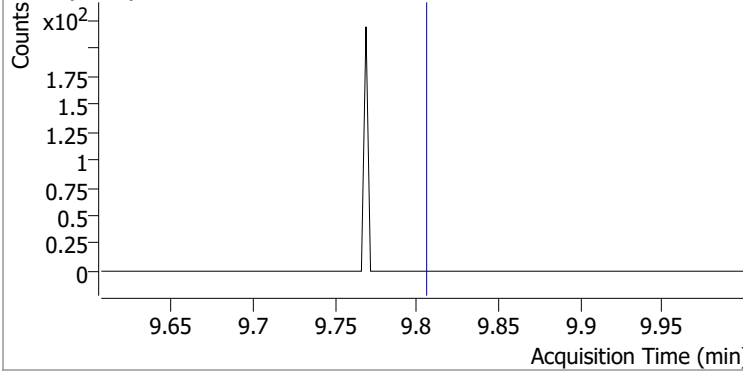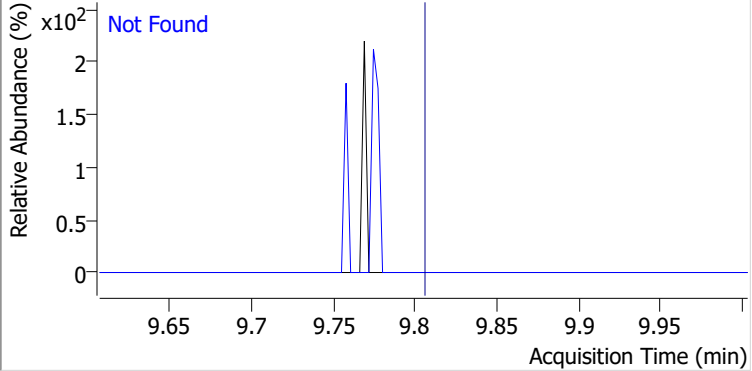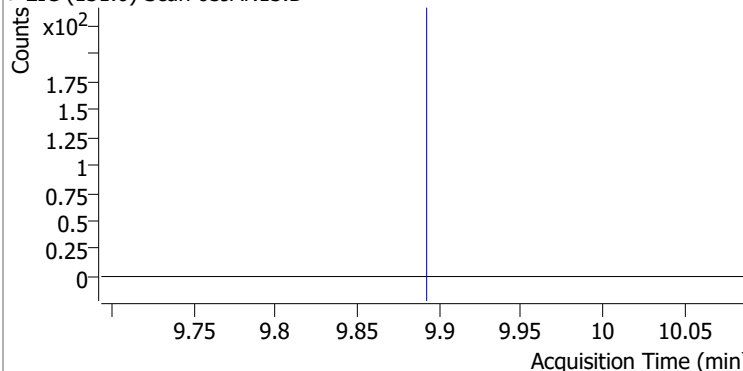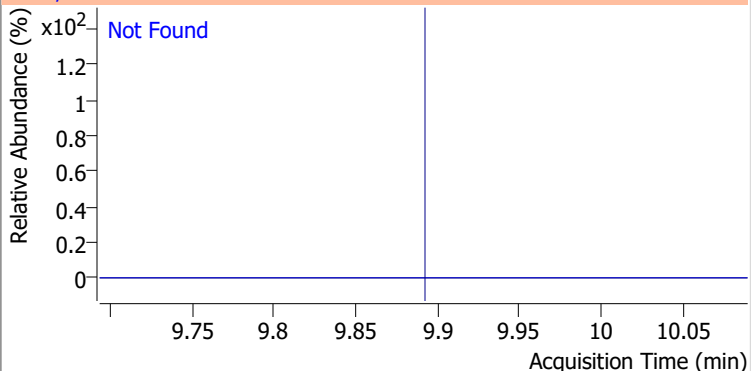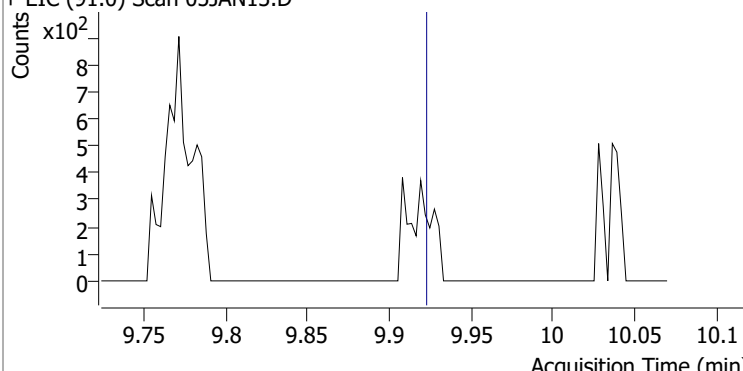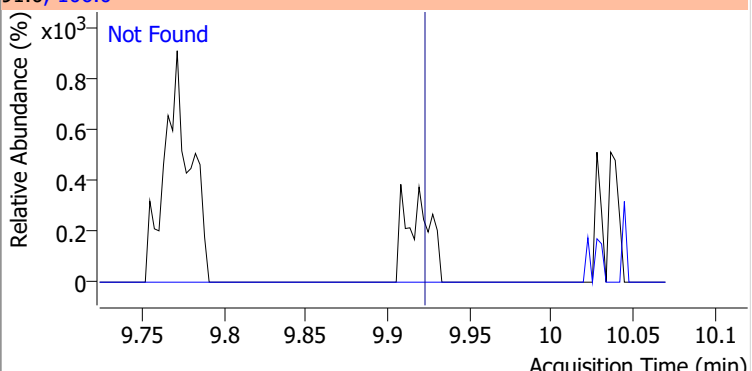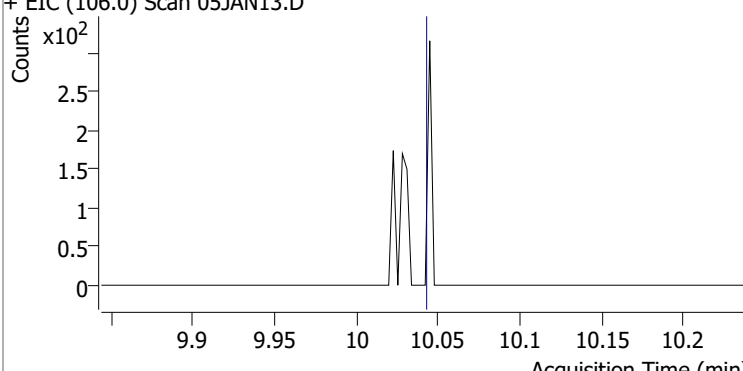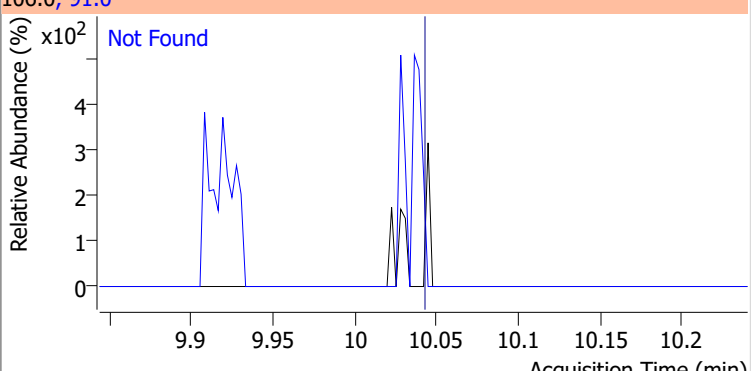
| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--|--|--------|--------------|-----------|
| Chlorobenzene | N.D. | 9.80 | 114.0 | 32.1 |
| + EIC (112.0) Scan 05JAN13.D | | | 112.0, 114.0 | |
|  |  | | | |
| 1,1,1,2-Tetrachloroethane | N.D. | 9.89 | 133.0 | 98.6 |
| + EIC (131.0) Scan 05JAN13.D | | | 131.0, 133.0 | |
|  |  | | | |
| Ethylbenzene | N.D. | 9.92 | 106.0 | 31.1 |
| + EIC (91.0) Scan 05JAN13.D | | | 91.0, 106.0 | |
|  |  | | | |
| m+p-Xylenes | N.D. | 10.04 | 91.0 | 201.4 |
| + EIC (106.0) Scan 05JAN13.D | | | 106.0, 91.0 | |
|  |  | | | |









Quantitation Results Report (QT Reviewed)

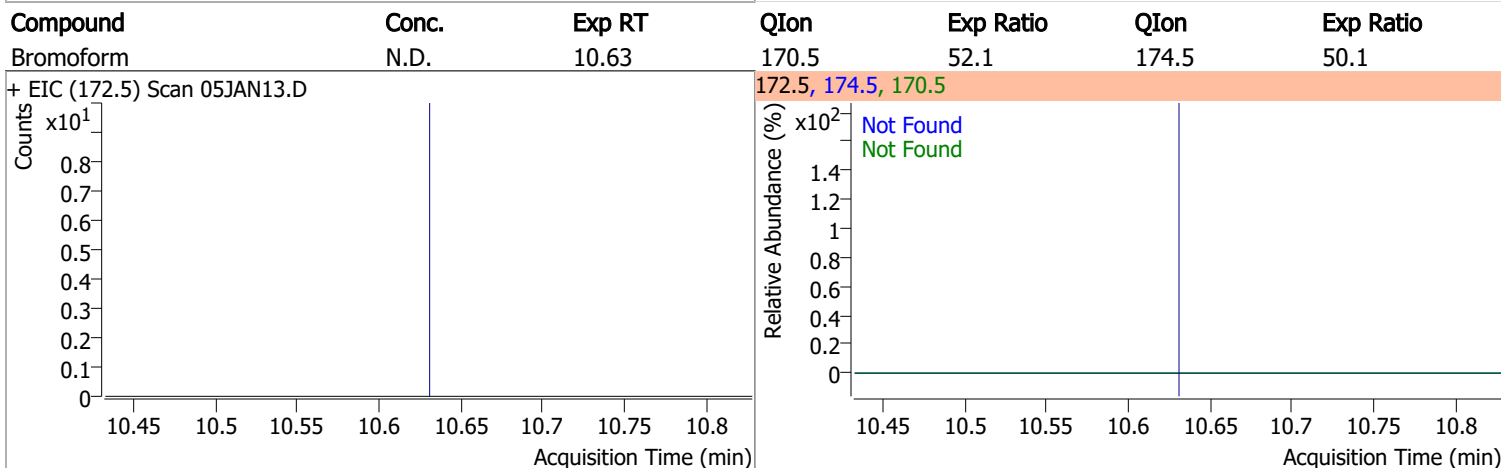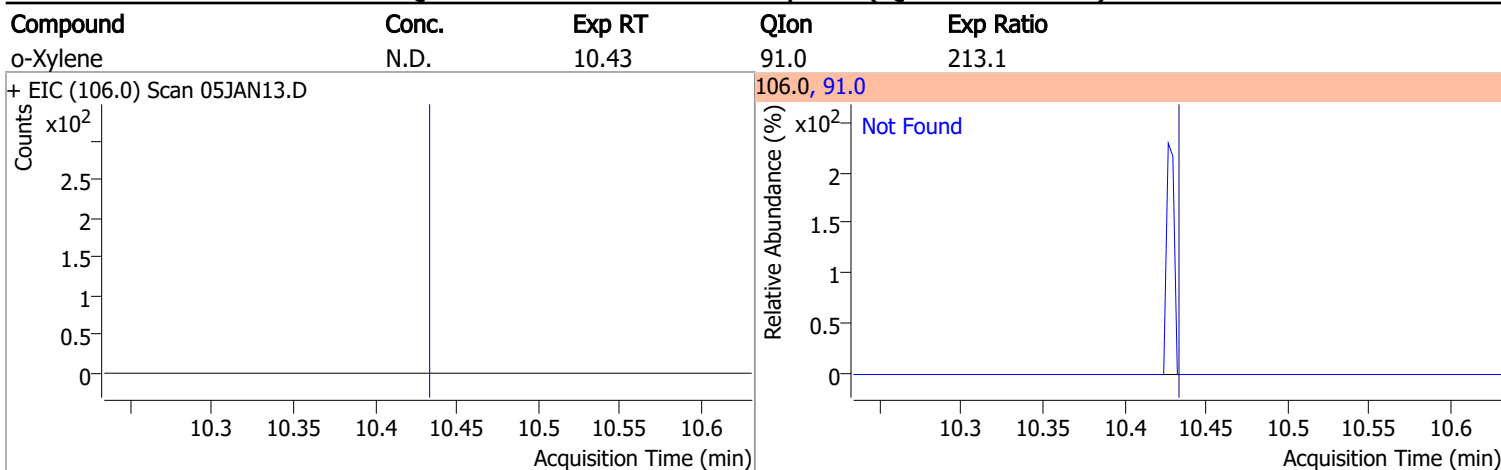









| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 265.3424 | 10.95 | 0.00 | 210682 | 174.0 | 95.8 | 61.7 | 121.7 |
| | | | | | 176.0 | 94.2 | 60.6 | 120.6 |



Quantitation Results Report (QT Reviewed)

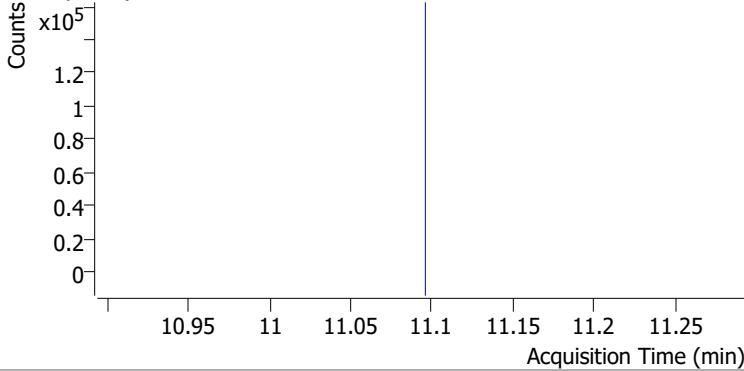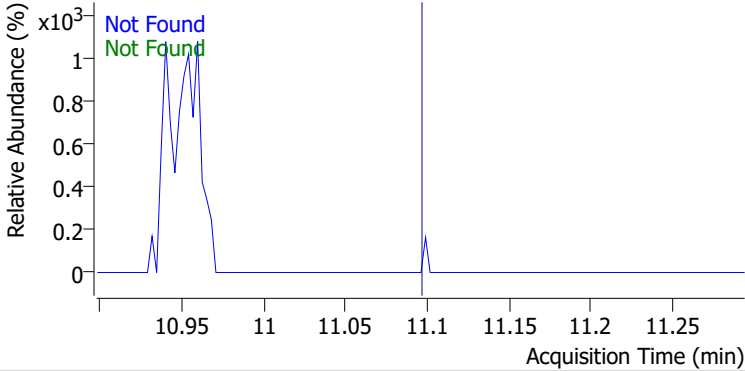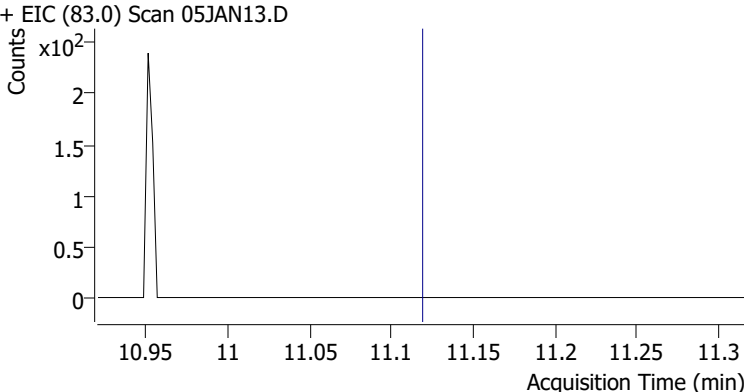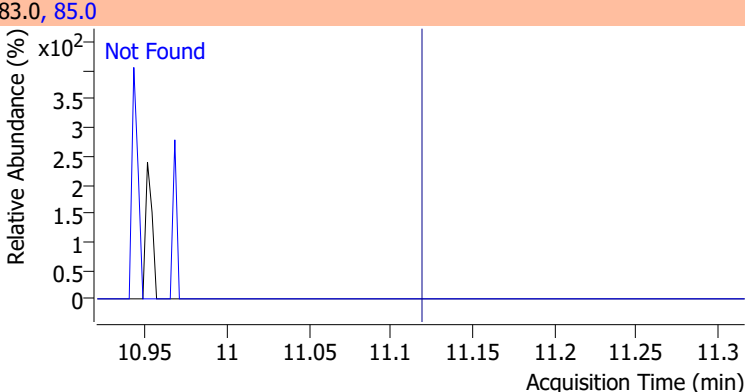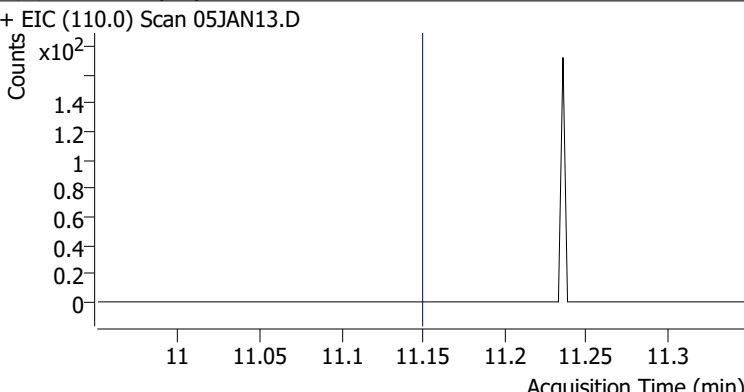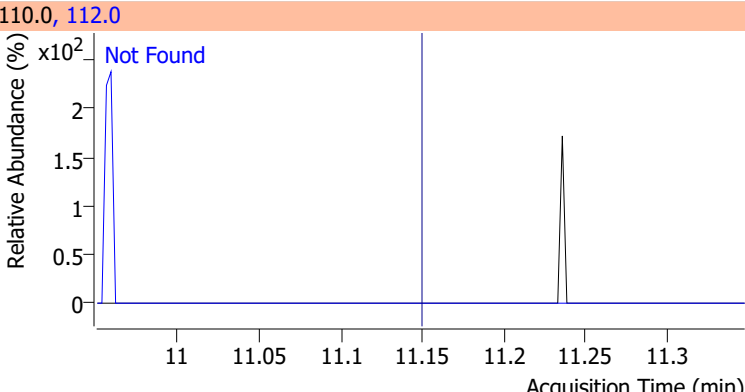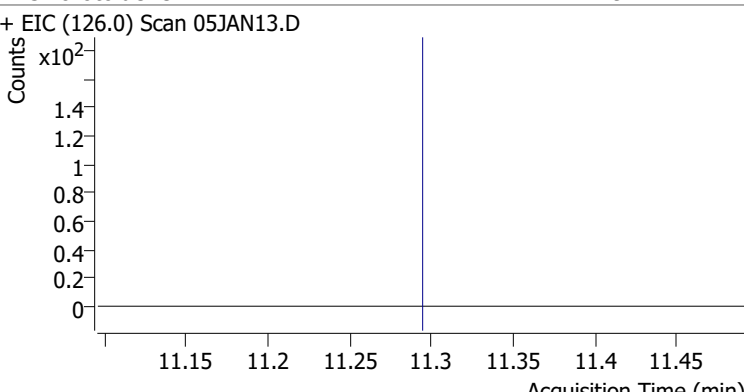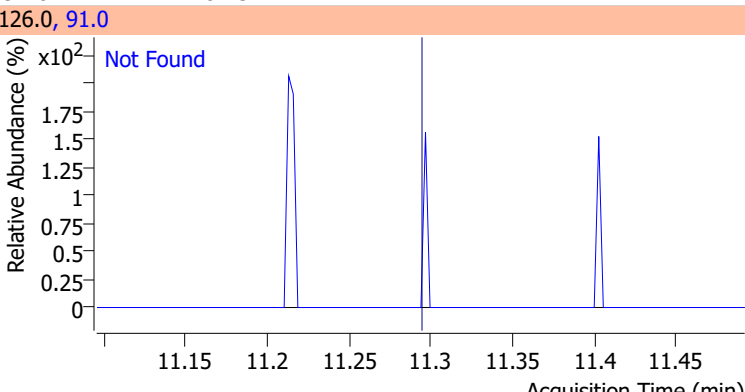
| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--|-------|--------|--|-----------|-------|-----------|
| Bromobenzene | N.D. | 11.09 | 77.0 | 145.7 | 158.0 | 96.5 |
| + EIC (156.0) Scan 05JAN13.D ***NO DATA POINTS*** | | | 156.0, 77.0, 158.0 | | | |
|  | | |  | | | |
| 1,1,2,2-Tetrachloroethane | N.D. | 11.12 | 85.0 | 66.2 | | |
| + EIC (83.0) Scan 05JAN13.D | | | 83.0, 85.0 | | | |
|  | | |  | | | |
| 1,2,3-Trichloropropane | N.D. | 11.15 | 112.0 | 63.5 | | |
| + EIC (110.0) Scan 05JAN13.D | | | 110.0, 112.0 | | | |
|  | | |  | | | |
| 2-Chlorotoluene | N.D. | 11.29 | 91.0 | 282.3 | | |
| + EIC (126.0) Scan 05JAN13.D | | | 126.0, 91.0 | | | |
|  | | |  | | | |

Quantitation Results Report (QT Reviewed)
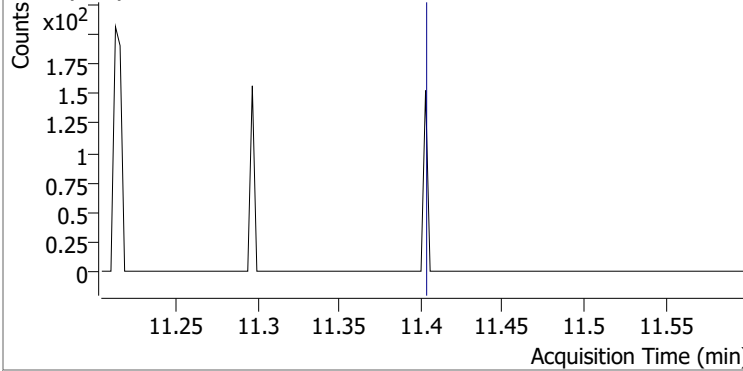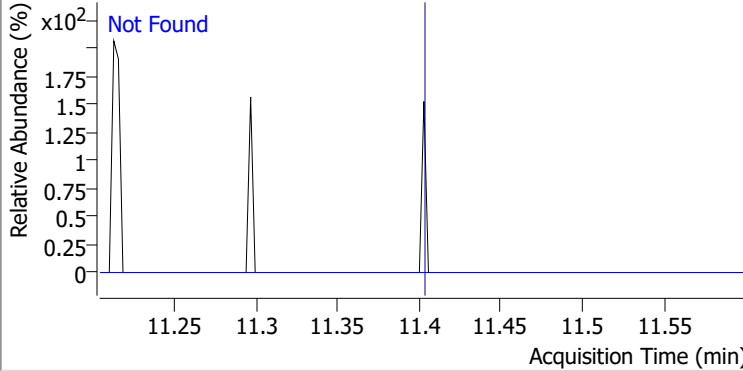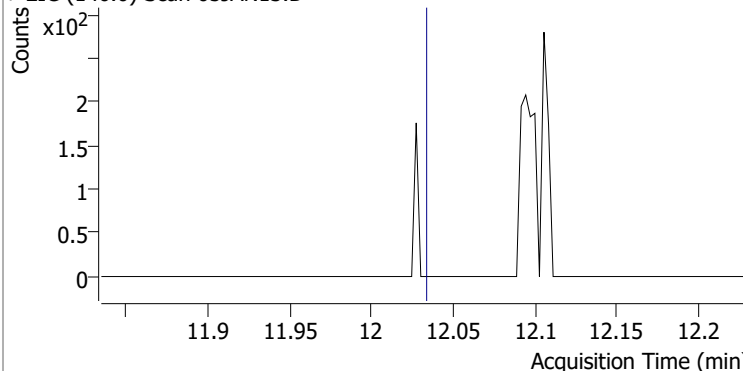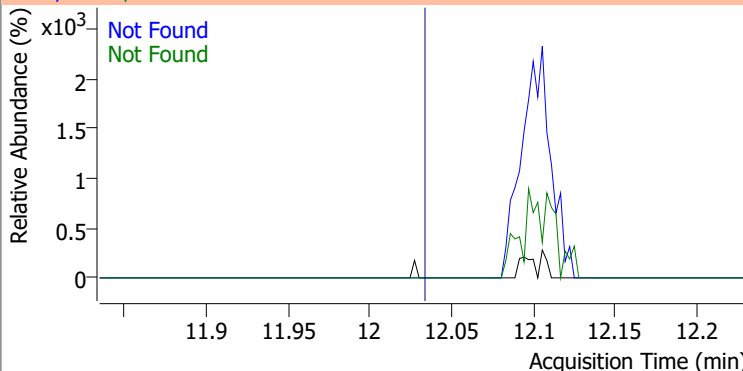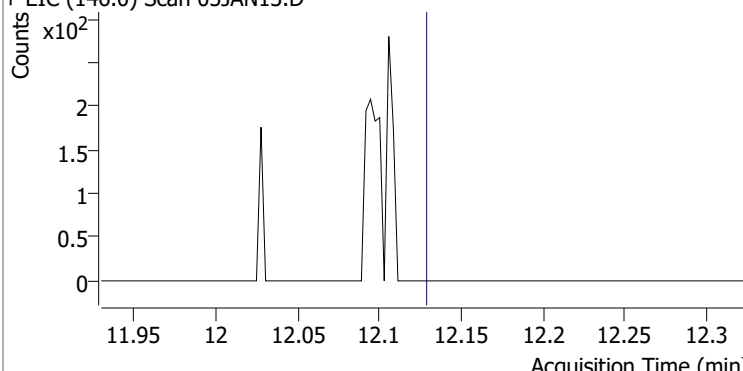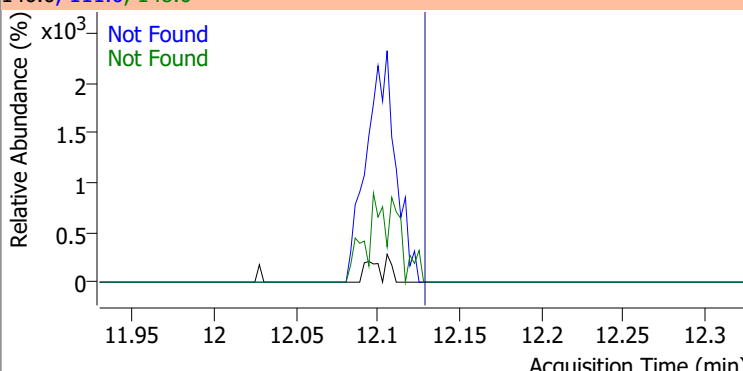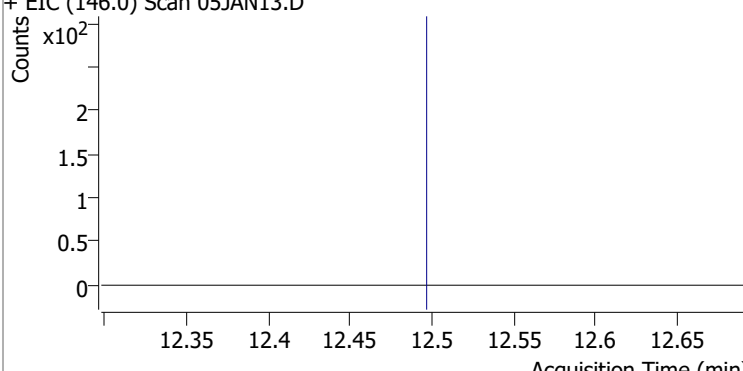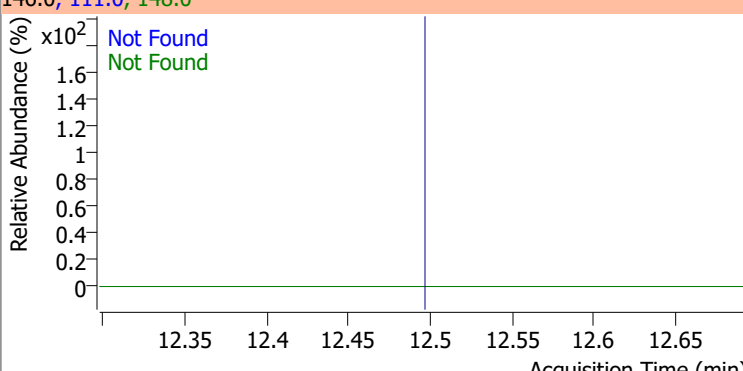
| Compound | Conc. | Exp RT | QIon | Exp Ratio | | |
|--|-------|--------|--|-----------|------|-----------|
| 4-Chlorotoluene | N.D. | 11.40 | 126.0 | 31.7 | | |
| + EIC (91.0) Scan 05JAN13.D | | | 91.0, 126.0 | | | |
|  | | |  | | | |
| 1,3-Dichlorobenzene | N.D. | 12.03 | 148.0 | 63.6 | QIon | Exp Ratio |
| + EIC (146.0) Scan 05JAN13.D | | | 146.0, 111.0, 148.0 | | | |
|  | | |  | | | |
| 1,4-Dichlorobenzene | N.D. | 12.13 | 148.0 | 63.1 | QIon | Exp Ratio |
| + EIC (146.0) Scan 05JAN13.D | | | 146.0, 111.0, 148.0 | | | |
|  | | |  | | | |
| 1,2-Dichlorobenzene | N.D. | 12.49 | 148.0 | 63.9 | QIon | Exp Ratio |
| + EIC (146.0) Scan 05JAN13.D | | | 146.0, 111.0, 148.0 | | | |
|  | | |  | | | |

Quantitation Results Report (QT Reviewed)

| | | | |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File | 05JAN14.D | Operator | MSC |
| Acq. Method | 5975CACQF.M | Acq. Date-Time | 1/5/2022 4:00:32 PM |
| Sample Name | B22010002-001F | Instrument | VOA5975C |
| Vial | 14 | Multiplier | 1.00 |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m | Comment | |
| Tune File | BFB_Atune3.u | Tune Date | 10/11/2021 4:02:00 PM |
| Batch Name | VG010522_8260B.batch.bin | Last Calib Update | 2/28/2022 2:48:47 PM |
| Ref Library | \\MASSHUNTER\Org\Library\NIST129K.l | | |







| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|----------------------|-------|----------|
| Internal Standards | | | | | | |
| M Fluorobenzene | 6.618 | 96.0 | 708497 | 250.0000 | ng | -0.006 |
| M Chlorobenzene-d5 | 9.772 | 82.0 | 279384 | 250.0000 | ng | 0.000 |
| M 1,4-Dichlorobenzene-d4 | 12.100 | 152.0 | 224639 | 250.0000 | ng | 0.000 |
| System Monitoring Compounds | | | | | | |
| S Dibromofluoromethane | 5.845 | 113.0 | 185929 | 278.5553 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 80.0 - 119.0% | | | Recovery = 111.42% | | |
| S 1,2-Dichloroethane-d4 | 6.233 | 67.0 | 85127 | 295.2707 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 81.0 - 118.0% | | | Recovery = 118.11% * | | |
| S Toluene-d8 | 8.319 | 98.0 | 711005 | 264.0896 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 89.0 - 112.0% | | | Recovery = 105.64% | | |
| S p-Bromofluorobenzene | 10.951 | 95.0 | 217356 | 264.1124 | ng | -0.003 |
| Spiked Amount: 250.000 | Range: 85.0 - 114.0% | | | Recovery = 105.64% | | |
| Target Compounds | | | | | | |
| T Dichlorodifluoromethane | 0.000 | | 0 | N.D. | | |
| T Chloromethane | 1.414 | 50.0 | 612 | 0.5433 | ng | m 87 |
| T Vinyl chloride | 0.000 | | 0 | N.D. | | |
| T Bromomethane | 0.000 | | 0 | N.D. | | |
| T Chloroethane | 0.000 | | 0 | N.D. | | |
| T Trichlorofluoromethane | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methylene chloride | 3.336 | 49.0 | 0 | | ng | md 1 |
| T trans-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methyl tert-butyl ether (MTBE) | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloroethane | 0.000 | | 0 | N.D. | | |
| T 2,2-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T cis-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methyl ethyl ketone | 0.000 | | 0 | N.D. | | |
| T Bromochloromethane | 0.000 | | 0 | N.D. | | |
| T Chloroform | 5.647 | 83.0 | 2570 | 1.9054 | ng | m 96 |

Quantitation Results Report (QT Reviewed)

| Compound | RT | QIon | Resp. | Conc. | Units | | Dev(Min) |
|-----------------------------|--------|-------|-------|---------|-------|----|----------|
| T 1,1,1-Trichloroethane | 0.000 | | 0 | N.D. | | | |
| T Carbon tetrachloride | 0.000 | | 0 | N.D. | | | |
| T 1,1-Dichloropropene | 0.000 | | 0 | N.D. | | | |
| T Benzene | 6.278 | 78.0 | 357 | 0.1266 | ng | m | 90 |
| T 1,2-Dichloroethane | 0.000 | | 0 | N.D. | | | |
| T Trichloroethene | 0.000 | | 0 | N.D. | | | |
| T 1,2-Dichloropropane | 0.000 | | 0 | N.D. | | | |
| T Dibromomethane | 0.000 | | 0 | N.D. | | | |
| T Bromodichloromethane | 7.591 | 83.0 | 1414 | 1.6353 | ng | m | 89 |
| T cis-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | | |
| T Toluene | 8.386 | 92.0 | 0 | | ng | md | 1 |
| T trans-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | | |
| T 1,1,2-Trichloroethane | 0.000 | | 0 | N.D. | | | |
| T Tetrachloroethene | 0.000 | | 0 | N.D. | | | |
| T 1,3-Dichloropropane | 0.000 | | 0 | N.D. | | | |
| T Chlorodibromomethane | 9.203 | 129.0 | 3282 | 5.7950 | ng | m | 94 |
| T 1,2-Dibromoethane | 0.000 | | 0 | N.D. | | | |
| T Chlorobenzene | 0.000 | | 0 | N.D. | | | |
| T 1,1,1,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | | |
| T Ethylbenzene | 9.928 | 91.0 | 333 | 0.0965 | ng | m | 74 |
| T m+p-Xylenes | 10.039 | 106.0 | 0 | | ng | md | 1 |
| T o-Xylene | 10.421 | 106.0 | 2546 | 2.1312 | ng | | 88 |
| T Styrene | 0.000 | | 0 | N.D. | | | |
| T Bromoform | 10.628 | 172.5 | 4757 | 16.5483 | ng | | 95 |
| T Bromobenzene | 0.000 | | 0 | N.D. | | | |
| T 1,1,2,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | | |
| T 1,2,3-Trichloropropane | 0.000 | | 0 | N.D. | | | |
| T 2-Chlorotoluene | 0.000 | | 0 | N.D. | | | |
| T 4-Chlorotoluene | 11.392 | 91.0 | 0 | | ng | md | 1 |
| T 1,3-Dichlorobenzene | 0.000 | | 0 | N.D. | | | |
| T 1,4-Dichlorobenzene | 0.000 | | 0 | N.D. | | | |
| T 1,2-Dichlorobenzene | 0.000 | | 0 | N.D. | | | |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)

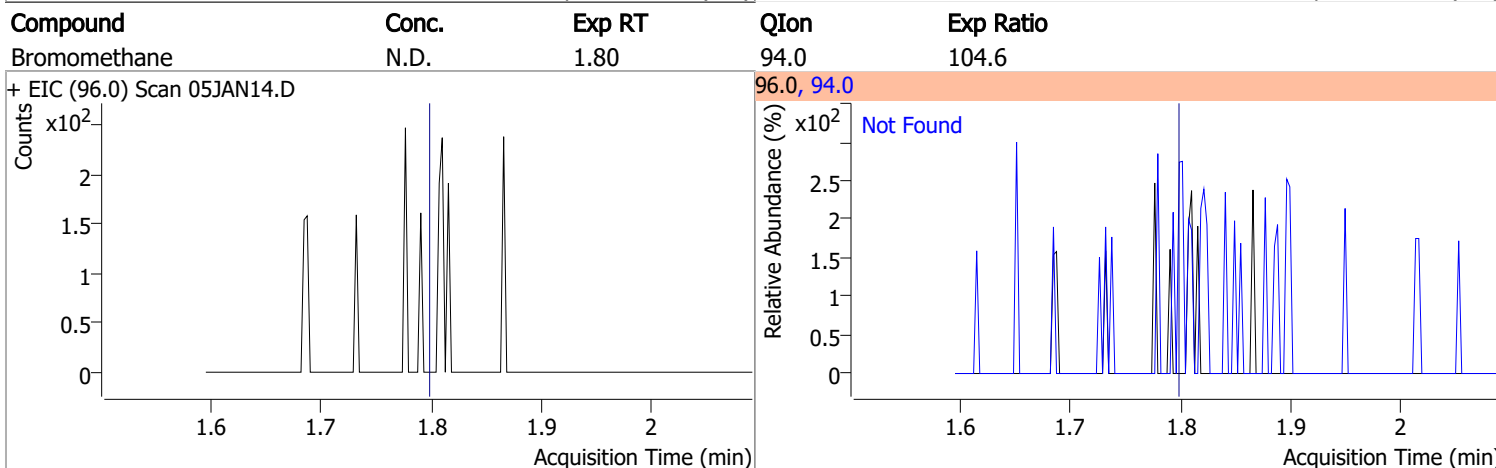


Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------|-------|--------|------|-----------|
| Chloroethane | N.D. | 1.89 | 66.0 | 30.1 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|------------------------|-------|--------|-------|-----------|
| Trichlorofluoromethane | N.D. | 2.14 | 103.0 | 64.2 |











| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethene | N.D. | 2.70 | 61.0 | 180.3 | 63.0 | 56.7 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|-------|----|----------|-------|------|--------|-------|-------|
| Methylene chloride | | 0 | | 0 | 84.0 | | 36.9 | 96.9 |
| | | | | | 86.0 | | 14.3 | 74.3 |




Quantitation Results Report (QT Reviewed)

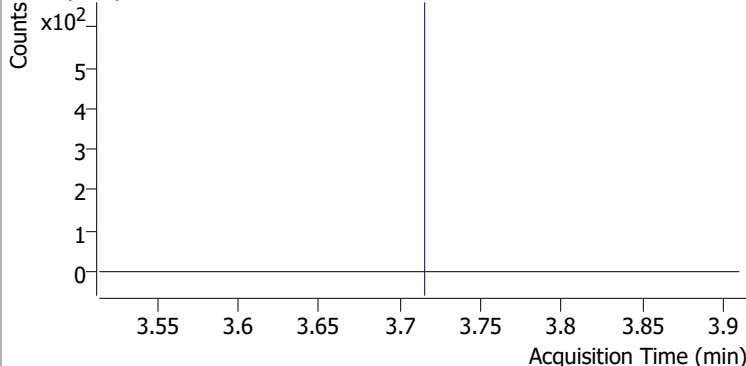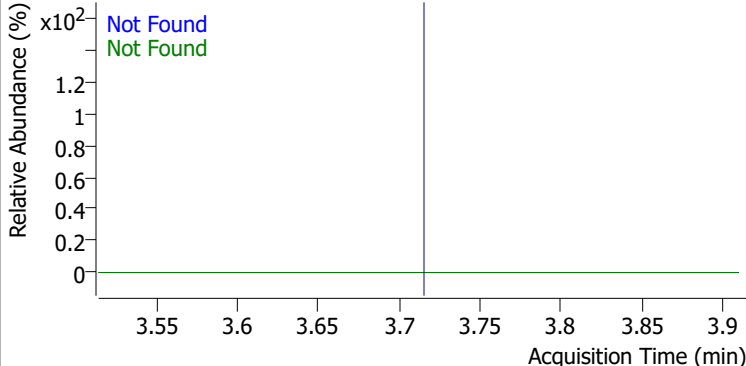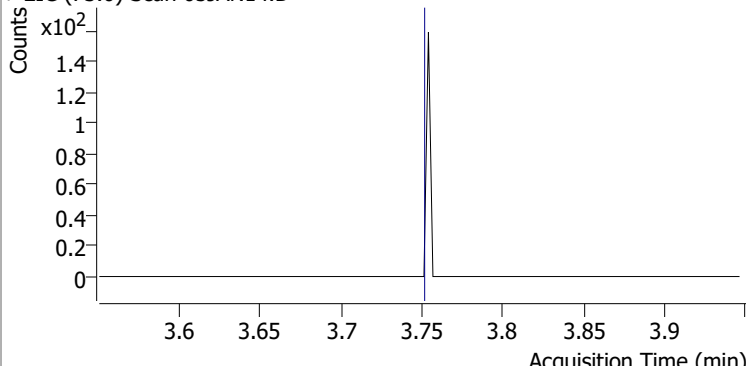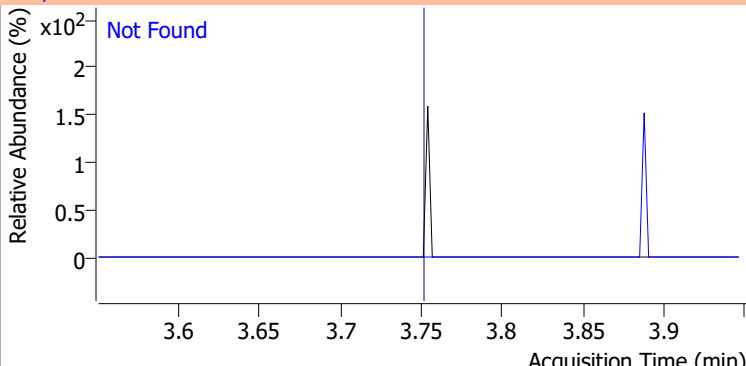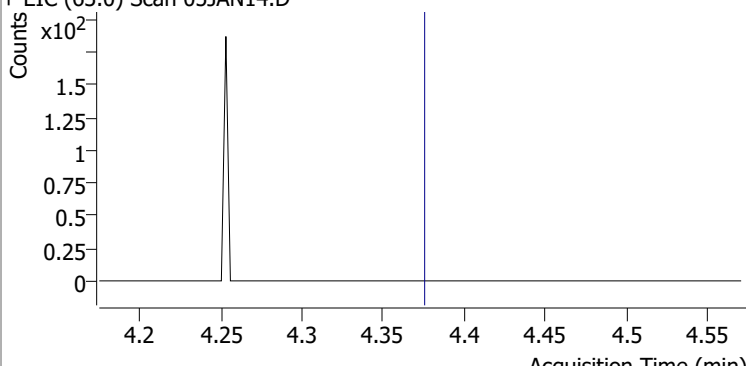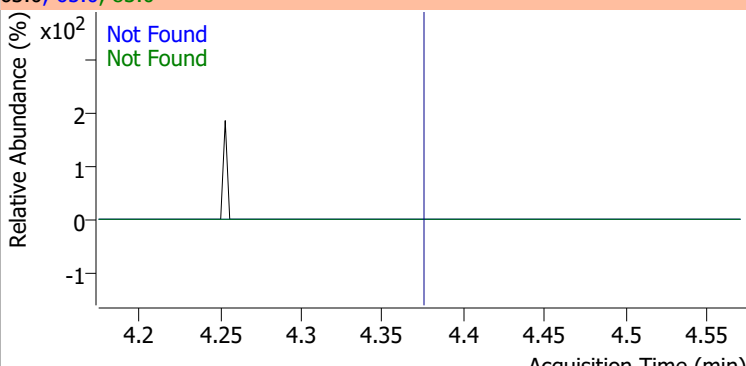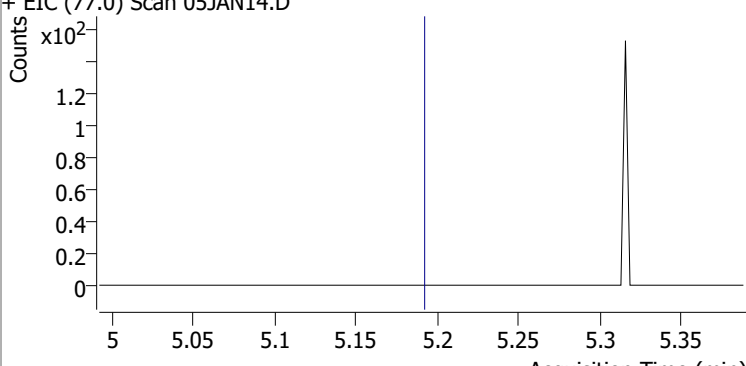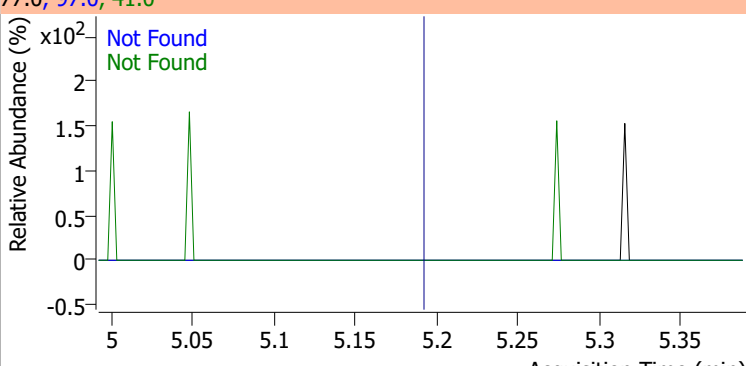
| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--|-------|--------|--|-----------|------|-----------|
| trans-1,2-Dichloroethene | N.D. | 3.72 | 61.0 | 153.9 | 98.0 | 65.7 |
| + EIC (96.0) Scan 05JAN14.D | | | 96.0, 61.0, 98.0 | | | |
|  | | |  | | | |
| Methyl tert-butyl ether (MTBE) | N.D. | 3.75 | 57.0 | 24.6 | | |
| + EIC (73.0) Scan 05JAN14.D | | | 73.0, 57.0 | | | |
|  | | |  | | | |
| 1,1-Dichloroethane | N.D. | 4.38 | 65.0 | 32.1 | 83.0 | 13.7 |
| + EIC (63.0) Scan 05JAN14.D | | | 63.0, 65.0, 83.0 | | | |
|  | | |  | | | |
| 2,2-Dichloropropane | N.D. | 5.20 | 41.0 | 66.5 | 97.0 | 23.2 |
| + EIC (77.0) Scan 05JAN14.D | | | 77.0, 97.0, 41.0 | | | |
|  | | |  | | | |

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|------------------------|-------|--------|------|-----------|------|-----------|
| cis-1,2-Dichloroethene | N.D. | 5.22 | 61.0 | 167.2 | 98.0 | 67.3 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| Methyl ethyl ketone | N.D. | 5.28 | 72.0 | 21.3 |







| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|
| Bromochloromethane | N.D. | 5.52 | 49.0 | 182.9 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|--------|------|----------|----------|------|--------|-------|-------|
| Chloroform | 1.9054 | 5.65 | -0.01 | 2570 (m) | 85.0 | 68.9 | 36.0 | 96.0 |




Quantitation Results Report (QT Reviewed)

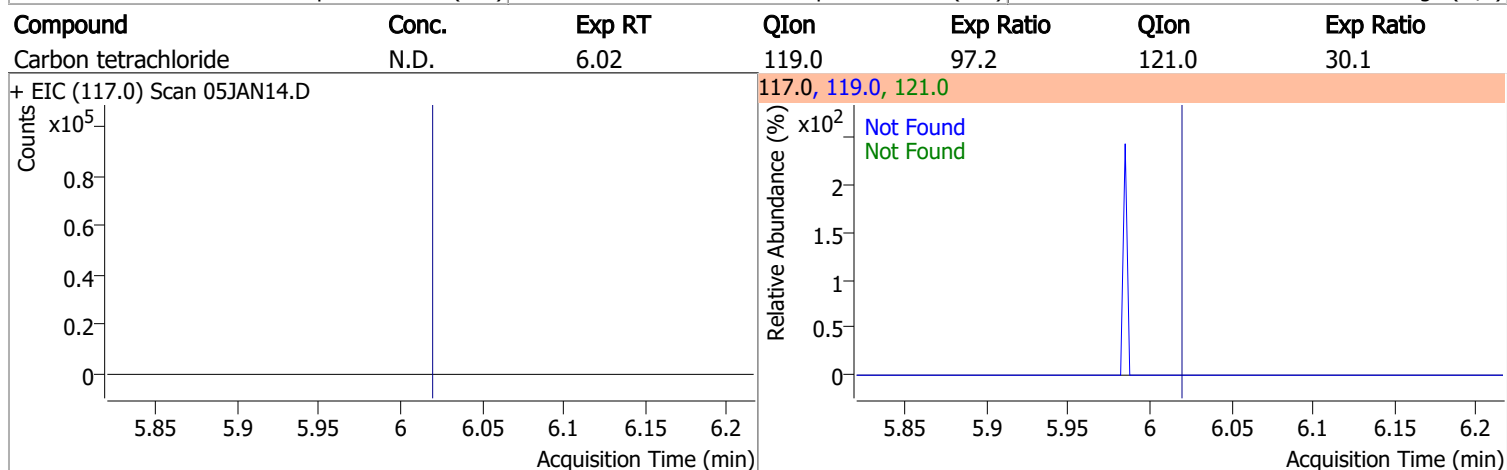


Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 295.2707 | 6.23 | 0.00 | 85127 | 65.0 | 196.2 | 166.5 | 226.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|--------|------|----------|---------|------|--------|-------|-------|
| Benzene | 0.1266 | 6.28 | 0.00 | 357 (m) | 77.0 | 18.7 | 0.0 | 53.5 |







| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,2-Dichloroethane | N.D. | 6.32 | 64.0 | 29.9 | 98.0 | 7.6 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------|-------|--------|-------|-----------|------|-----------|
| Trichloroethene | N.D. | 7.03 | 130.0 | 101.5 | 97.0 | 64.1 |




Quantitation Results Report (QT Reviewed)

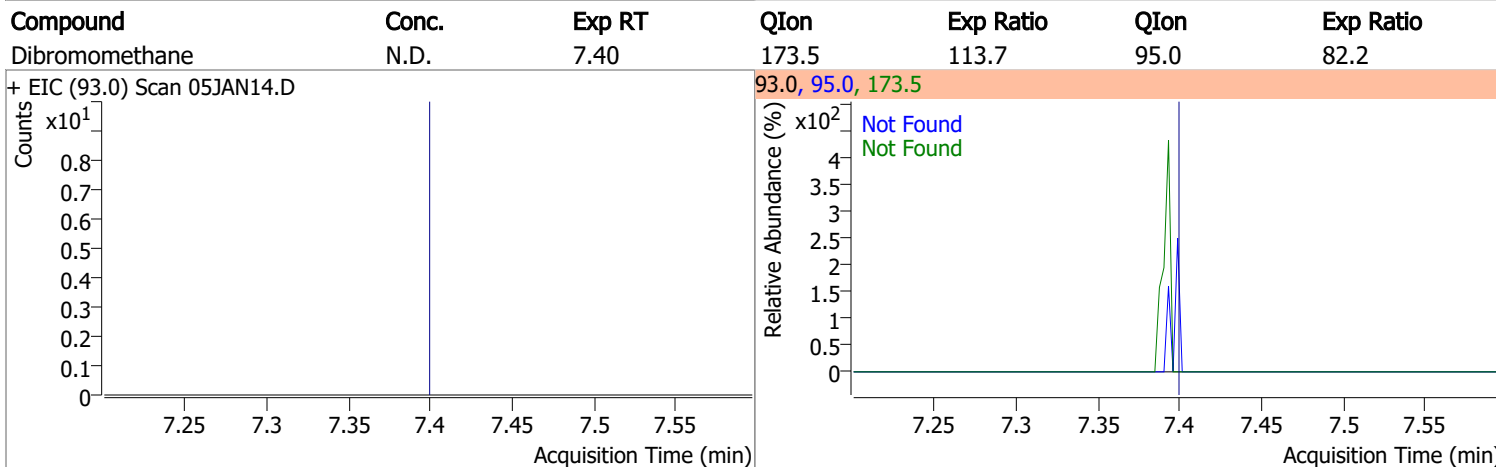


Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 264.0896 | 8.32 | 0.00 | 711005 | 100.0 | 64.5 | 34.4 | 94.4 |
| | | | | | 99.0 | 9.6 | 0.0 | 39.6 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|-------|----|----------|-------|------|--------|-------|-------|
| Toluene | 0 | 0 | 0 | 0 | 91.0 | | 145.8 | 205.8 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,3-Dichloropropene | N.D. | 8.64 | 39.0 | 53.4 | 77.0 | 32.4 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------------|-------|--------|------|-----------|------|-----------|
| 1,1,2-Trichloroethane | N.D. | 8.82 | 97.0 | 114.6 | 85.0 | 67.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-------------------|-------|--------|-------|-----------|-------|-----------|
| Tetrachloroethene | N.D. | 8.94 | 165.8 | 128.6 | 129.0 | 91.5 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| 1,3-Dichloropropane | N.D. | 8.98 | 78.0 | 32.9 |







| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|--------|------|----------|----------|-------|--------|-------|-------|
| Chlorodibromomethane | 5.7950 | 9.20 | 0.00 | 3282 (m) | 127.0 | 72.8 | 48.0 | 108.0 |







| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|-------------------|-------|--------|-------|-----------|
| 1,2-Dibromoethane | N.D. | 9.31 | 109.0 | 94.5 |











Quantitation Results Report (QT Reviewed)



Quantitation Results Report (QT Reviewed)

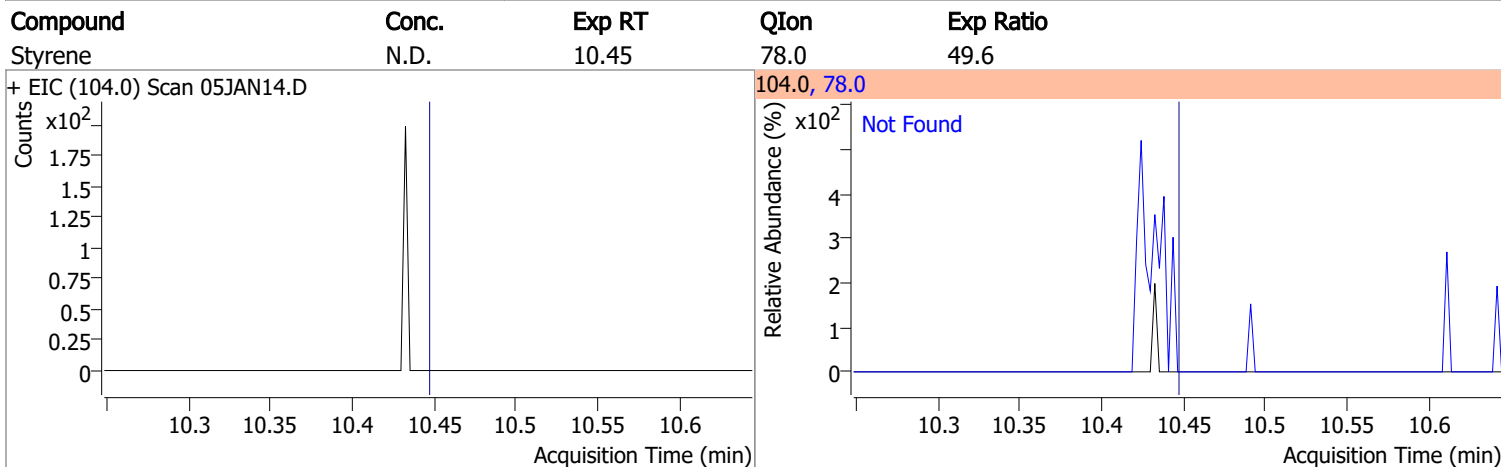


Quantitation Results Report (QT Reviewed)

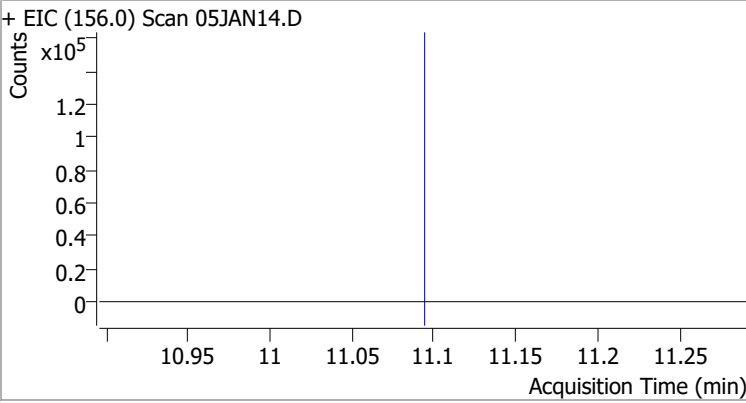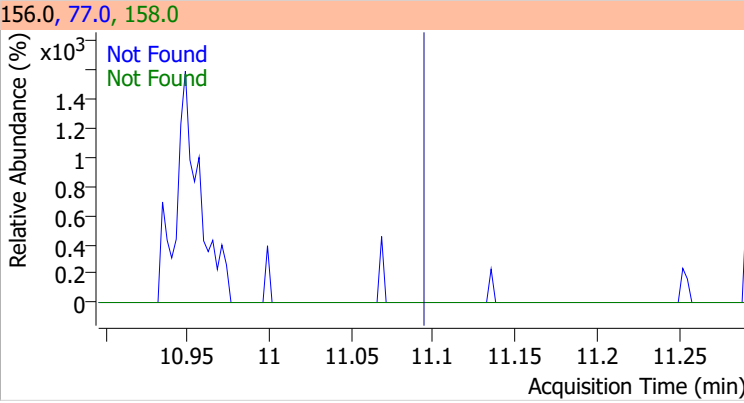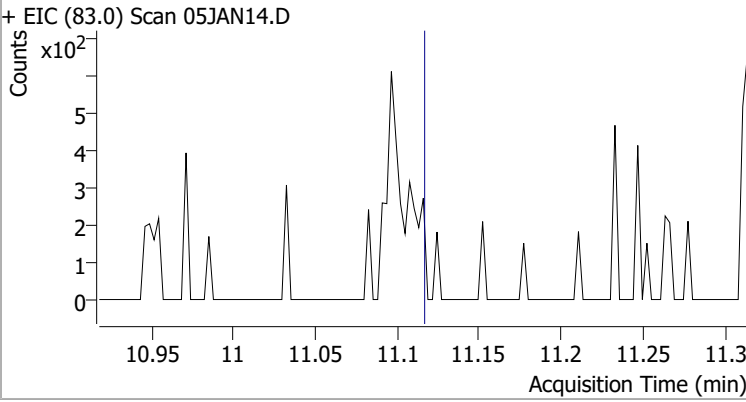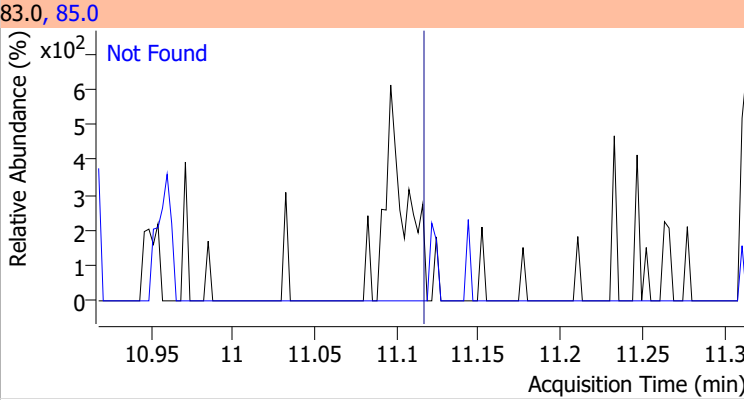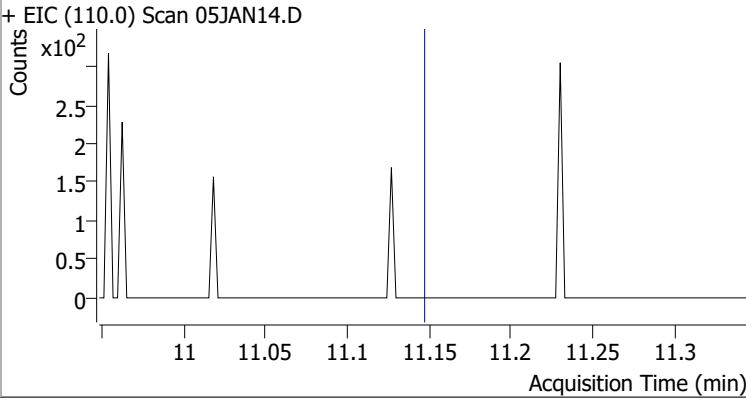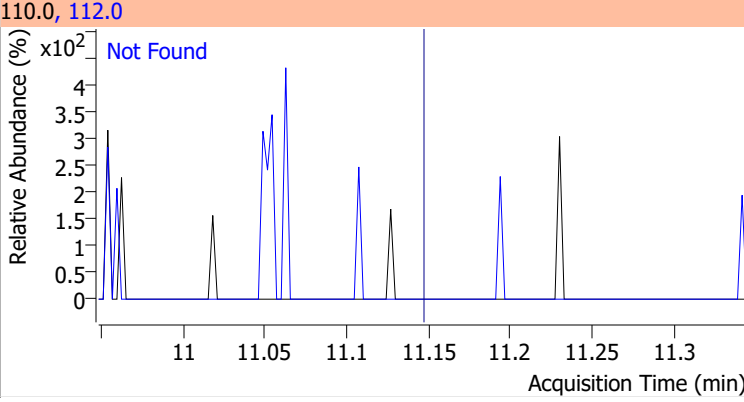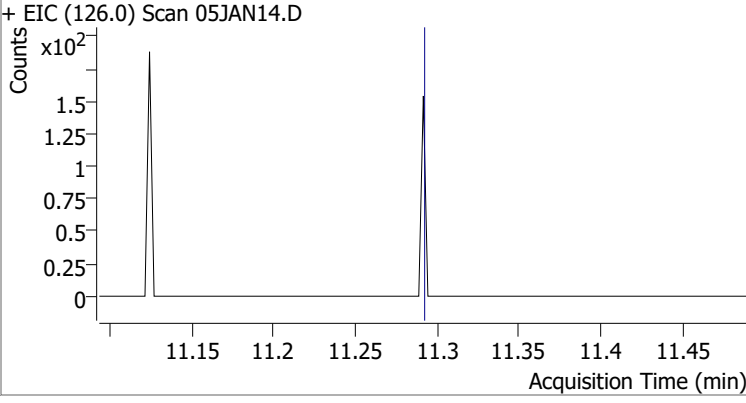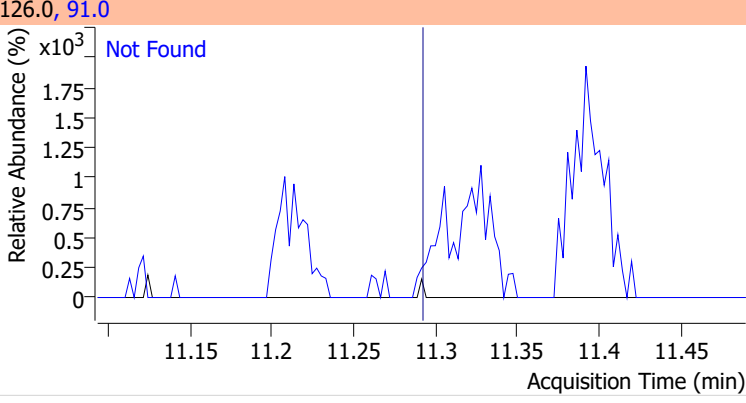
| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--|-------|--------|--|-----------|-------|-----------|
| Bromobenzene | N.D. | 11.09 | 77.0 | 145.7 | 158.0 | 96.5 |
| + EIC (156.0) Scan 05JAN14.D | | | 156.0, 77.0, 158.0 | | | |
|  | | |  | | | |
| 1,1,2,2-Tetrachloroethane | N.D. | 11.12 | 85.0 | 66.2 | | |
| + EIC (83.0) Scan 05JAN14.D | | | 83.0, 85.0 | | | |
|  | | |  | | | |
| 1,2,3-Trichloropropane | N.D. | 11.15 | 112.0 | 63.5 | | |
| + EIC (110.0) Scan 05JAN14.D | | | 110.0, 112.0 | | | |
|  | | |  | | | |
| 2-Chlorotoluene | N.D. | 11.29 | 91.0 | 282.3 | | |
| + EIC (126.0) Scan 05JAN14.D | | | 126.0, 91.0 | | | |
|  | | |  | | | |

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|-------|----|----------|-------|-------|--------|-------|-------|
| 4-Chlorotoluene | 0 | 0 | | 0 | 126.0 | | 1.7 | 61.7 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|-------|-----------|-------|-----------|
| 1,3-Dichlorobenzene | N.D. | 12.03 | 148.0 | 63.6 | 111.0 | 39.8 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|-------|-----------|-------|-----------|
| 1,4-Dichlorobenzene | N.D. | 12.13 | 148.0 | 63.1 | 111.0 | 39.1 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|-------|-----------|-------|-----------|
| 1,2-Dichlorobenzene | N.D. | 12.49 | 148.0 | 63.9 | 111.0 | 41.0 |



Quantitation Results Report (QT Reviewed)

| | | | |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File | 05JAN15.D | Operator | MSC |
| Acq. Method | 5975CACQF.M | Acq. Date-Time | 1/5/2022 4:27:50 PM |
| Sample Name | B22010002-002F | Instrument | VOA5975C |
| Vial | 15 | Multiplier | 1.00 |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m | Comment | |
| Tune File | BFB_Atune3.u | Tune Date | 10/11/2021 4:02:00 PM |
| Batch Name | VG010522_8260B.batch.bin | Last Calib Update | 2/28/2022 2:48:47 PM |
| Ref Library | \\MASSHUNTER\Org\Library\NIST129K.l | | |



| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|----------|----|------|-------|-------|-------|----------|
|----------|----|------|-------|-------|-------|----------|

Internal Standards

| | | | | | | |
|--------------------------|--------|-------|--------|----------|----|--------|
| M Fluorobenzene | 6.620 | 96.0 | 748274 | 250.0000 | ng | -0.003 |
| M Chlorobenzene-d5 | 9.774 | 82.0 | 290927 | 250.0000 | ng | 0.003 |
| M 1,4-Dichlorobenzene-d4 | 12.100 | 152.0 | 224022 | 250.0000 | ng | 0.000 |

System Monitoring Compounds

| | | | | | | |
|-------------------------|----------------------|-------|--------|--------------------|----|--------|
| S Dibromofluoromethane | 5.848 | 113.0 | 195751 | 277.6807 | ng | 0.003 |
| Spiked Amount: 250.000 | Range: 80.0 - 119.0% | | | Recovery = 111.07% | | |
| S 1,2-Dichloroethane-d4 | 6.230 | 67.0 | 88055 | 289.1908 | ng | -0.003 |
| Spiked Amount: 250.000 | Range: 81.0 - 118.0% | | | Recovery = 115.68% | | |
| S Toluene-d8 | 8.319 | 98.0 | 745560 | 265.9370 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 89.0 - 112.0% | | | Recovery = 106.37% | | |
| S p-Bromofluorobenzene | 10.951 | 95.0 | 222254 | 270.8078 | ng | -0.003 |
| Spiked Amount: 250.000 | Range: 85.0 - 114.0% | | | Recovery = 108.32% | | |

Target Compounds

| Compound | RT | QIon | Resp. | Conc. | Units | QValue |
|----------------------------------|-------|------|-------|--------|-------|--------|
| T Dichlorodifluoromethane | 0.000 | | 0 | N.D. | | |
| T Chloromethane | 1.397 | 50.0 | 529 | 0.4441 | ng | m 80 |
| T Vinyl chloride | 0.000 | | 0 | N.D. | | |
| T Bromomethane | 0.000 | | 0 | N.D. | | |
| T Chloroethane | 0.000 | | 0 | N.D. | | |
| T Trichlorofluoromethane | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methylene chloride | 3.327 | 49.0 | 658 | 0.5926 | ng | m 74 |
| T trans-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methyl tert-butyl ether (MTBE) | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloroethane | 0.000 | | 0 | N.D. | | |
| T 2,2-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T cis-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methyl ethyl ketone | 0.000 | | 0 | N.D. | | |
| T Bromochloromethane | 0.000 | | 0 | N.D. | | |
| T Chloroform | 5.647 | 83.0 | 2719 | 1.9088 | ng | 93 |


Quantitation Results Report (QT Reviewed)

| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|-----------------------------|--------|-------|-------|---------|-------|----------|
| T 1,1,1-Trichloroethane | 0.000 | | 0 | N.D. | | |
| T Carbon tetrachloride | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloropropene | 0.000 | | 0 | N.D. | | |
| T Benzene | 0.000 | | 0 | N.D. | | |
| T 1,2-Dichloroethane | 0.000 | | 0 | N.D. | | |
| T Trichloroethene | 0.000 | | 0 | N.D. | | |
| T 1,2-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T Dibromomethane | 0.000 | | 0 | N.D. | | |
| T Bromodichloromethane | 7.588 | 83.0 | 1705 | 1.8943 | ng m | 90 |
| T cis-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | |
| T Toluene | 0.000 | | 0 | N.D. | | |
| T trans-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | |
| T 1,1,2-Trichloroethane | 0.000 | | 0 | N.D. | | |
| T Tetrachloroethene | 0.000 | | 0 | N.D. | | |
| T 1,3-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T Chlorodibromomethane | 9.205 | 129.0 | 3071 | 5.2076 | ng | 100 |
| T 1,2-Dibromoethane | 0.000 | | 0 | N.D. | | |
| T Chlorobenzene | 0.000 | | 0 | N.D. | | |
| T 1,1,1,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | |
| T Ethylbenzene | 0.000 | | 0 | N.D. | | |
| T m+p-Xylenes | 0.000 | | 0 | N.D. | | |
| T o-Xylene | 0.000 | | 0 | N.D. | | |
| T Styrene | 0.000 | | 0 | N.D. | | |
| T Bromoform | 10.625 | 172.5 | 4407 | 15.3730 | ng | 93 |
| T Bromobenzene | 0.000 | | 0 | N.D. | | |
| T 1,1,2,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | |
| T 1,2,3-Trichloropropane | 0.000 | | 0 | N.D. | | |
| T 2-Chlorotoluene | 0.000 | | 0 | N.D. | | |
| T 4-Chlorotoluene | 0.000 | | 0 | N.D. | | |
| T 1,3-Dichlorobenzene | 0.000 | | 0 | N.D. | | |
| T 1,4-Dichlorobenzene | 0.000 | | 0 | N.D. | | |
| T 1,2-Dichlorobenzene | 0.000 | | 0 | N.D. | | |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|-------------------------|-------|--------|------|-----------|
| Dichlorodifluoromethane | N.D. | 1.24 | 87.0 | 32.3 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------|--------|------|----------|---------|------|--------|-------|-------|
| Chloromethane | 0.4441 | 1.40 | -0.01 | 529 (m) | 52.0 | 21.1 | 2.1 | 62.1 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------------|-------|--------|------|-----------|
| Vinyl chloride | N.D. | 1.50 | 64.0 | 29.9 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------|-------|--------|------|-----------|
| Bromomethane | N.D. | 1.80 | 94.0 | 104.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------|-------|--------|------|-----------|
| Chloroethane | N.D. | 1.89 | 66.0 | 30.1 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|------------------------|-------|--------|-------|-----------|
| Trichlorofluoromethane | N.D. | 2.14 | 103.0 | 64.2 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethene | N.D. | 2.70 | 61.0 | 180.3 | 63.0 | 56.7 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|--------|------|----------|---------|------|--------|-------|-------|
| Methylene chloride | 0.5926 | 3.33 | -0.01 | 658 (m) | 84.0 | 42.9 | 36.9 | 96.9 |
| | | | | | 86.0 | 32.0 | 14.3 | 74.3 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,2-Dichloroethene | N.D. | 3.72 | 61.0 | 153.9 | 98.0 | 65.7 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------------------|-------|--------|------|-----------|
| Methyl tert-butyl ether (MTBE) | N.D. | 3.75 | 57.0 | 24.6 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethane | N.D. | 4.38 | 65.0 | 32.1 | 83.0 | 13.7 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|------|-----------|
| 2,2-Dichloropropane | N.D. | 5.20 | 41.0 | 66.5 | 97.0 | 23.2 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|------------------------|-------|--------|------|-----------|------|-----------|
| cis-1,2-Dichloroethene | N.D. | 5.22 | 61.0 | 167.2 | 98.0 | 67.3 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| Methyl ethyl ketone | N.D. | 5.28 | 72.0 | 21.3 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|
| Bromochloromethane | N.D. | 5.52 | 49.0 | 182.9 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|--------|------|----------|-------|------|--------|-------|-------|
| Chloroform | 1.9088 | 5.65 | -0.01 | 2719 | 85.0 | 71.9 | 36.0 | 96.0 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------------|-------|--------|------|-----------|------|-----------|
| 1,1,1-Trichloroethane | N.D. | 5.83 | 99.0 | 64.7 | 61.0 | 48.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Dibromofluoromethane | 277.6807 | 5.85 | 0.00 | 195751 | 191.5 | 22.2 | 0.0 | 53.1 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|----------------------|-------|--------|-------|-----------|-------|-----------|
| Carbon tetrachloride | N.D. | 6.02 | 119.0 | 97.2 | 121.0 | 30.1 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|-------|-----------|------|-----------|
| 1,1-Dichloropropene | N.D. | 6.04 | 110.0 | 35.9 | 77.0 | 30.1 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 289.1908 | 6.23 | 0.00 | 88055 | 65.0 | 192.8 | 166.5 | 226.5 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------|-------|--------|------|-----------|
| Benzene | N.D. | 6.28 | 77.0 | 23.5 |







| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,2-Dichloroethane | N.D. | 6.32 | 64.0 | 29.9 | 98.0 | 7.6 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------|-------|--------|-------|-----------|------|-----------|
| Trichloroethene | N.D. | 7.03 | 130.0 | 101.5 | 97.0 | 64.1 |




Quantitation Results Report (QT Reviewed)

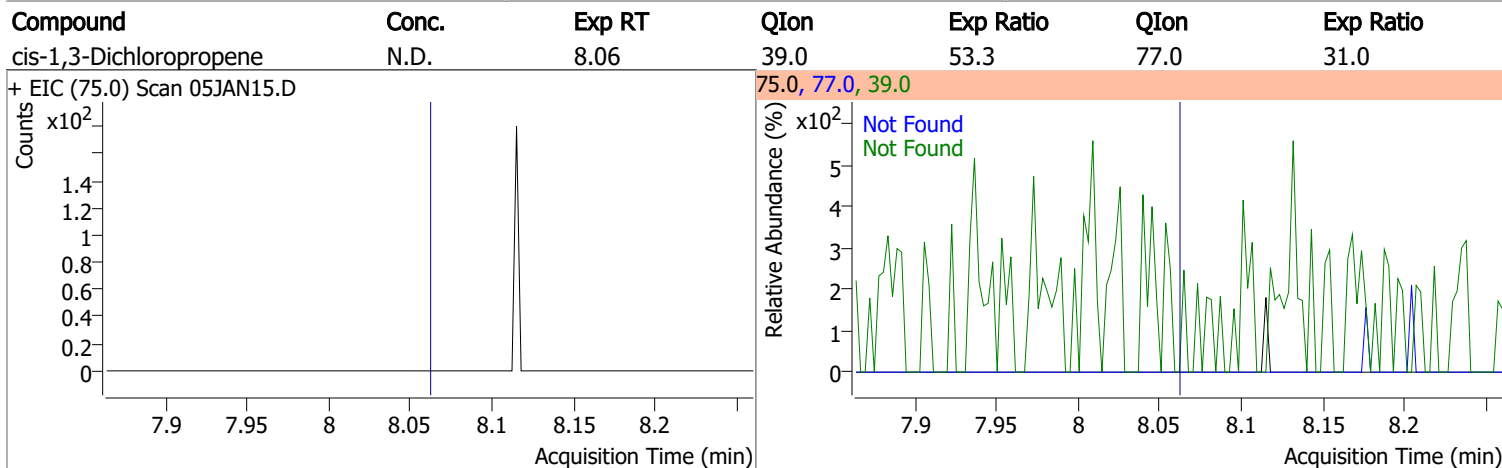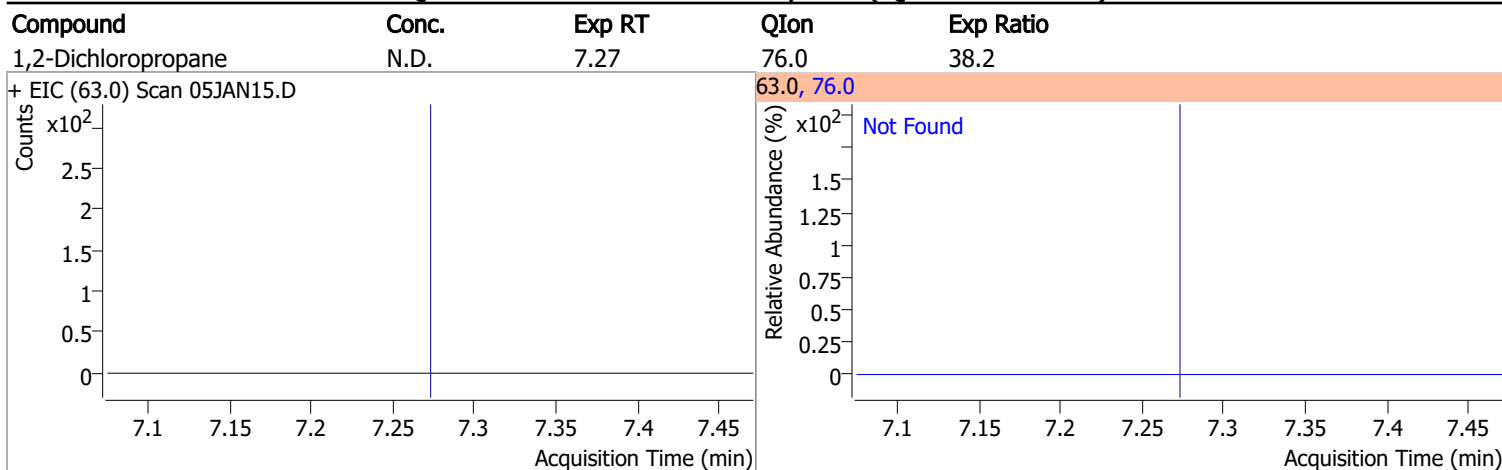


Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 265.9370 | 8.32 | 0.00 | 745560 | 100.0 | 64.6 | 34.4 | 94.4 |
| | | | | | 99.0 | 9.7 | 0.0 | 39.6 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------|-------|--------|------|-----------|
| Toluene | N.D. | 8.39 | 91.0 | 175.8 |







| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,3-Dichloropropene | N.D. | 8.64 | 39.0 | 53.4 | 77.0 | 32.4 |











| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------------|-------|--------|------|-----------|------|-----------|
| 1,1,2-Trichloroethane | N.D. | 8.82 | 97.0 | 114.6 | 85.0 | 67.6 |





Quantitation Results Report (QT Reviewed)

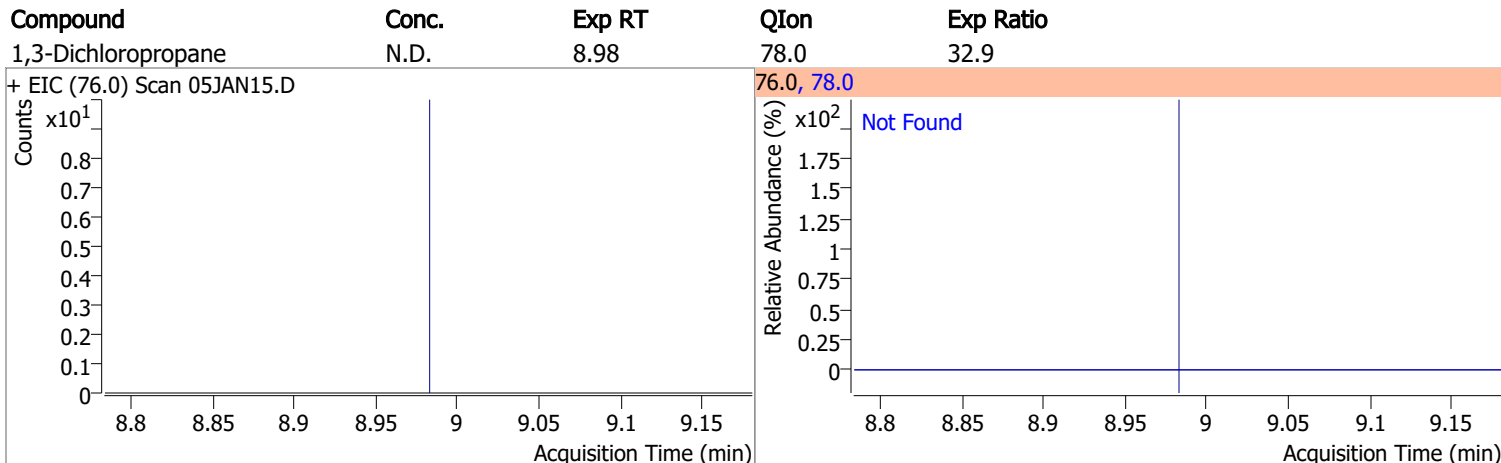


Quantitation Results Report (QT Reviewed)
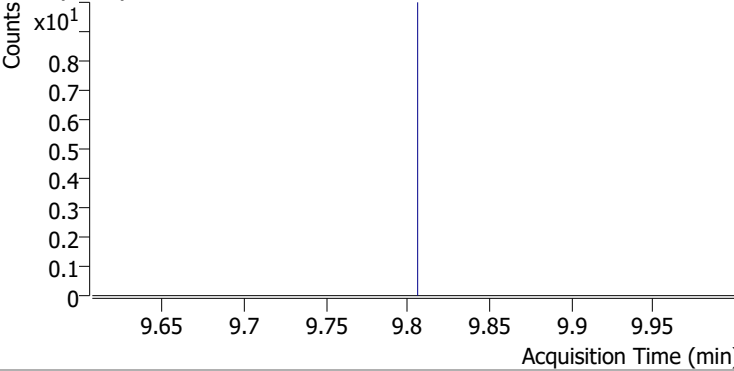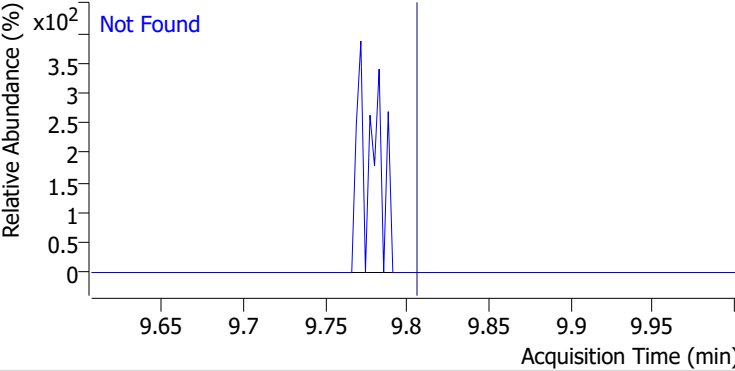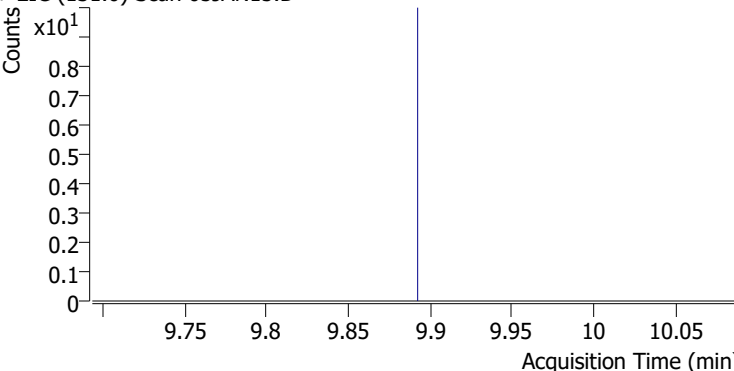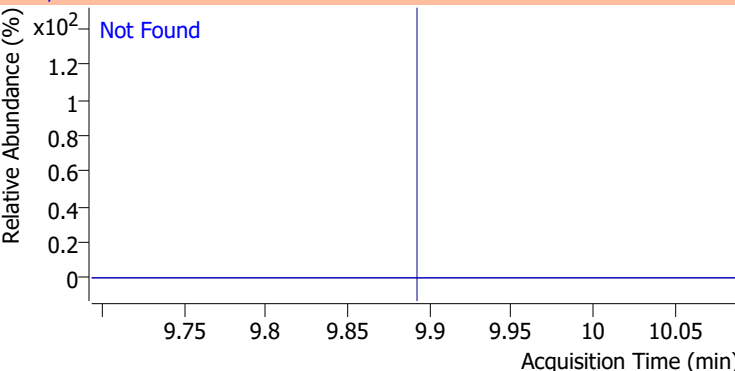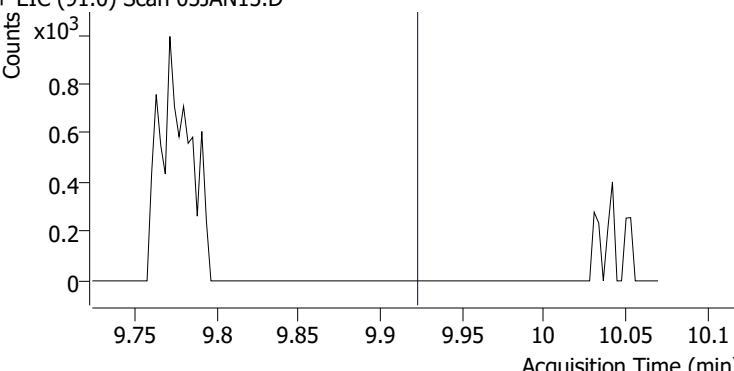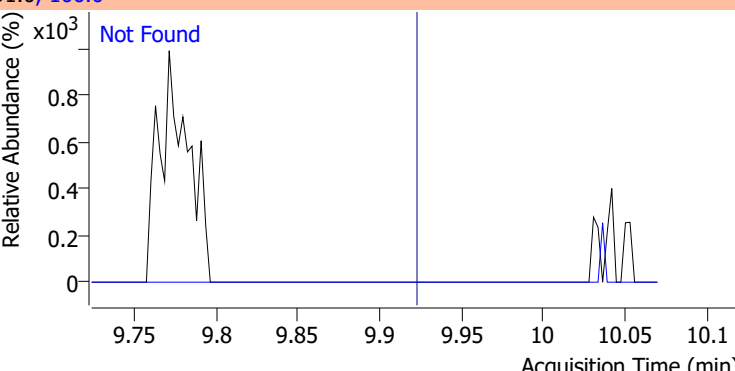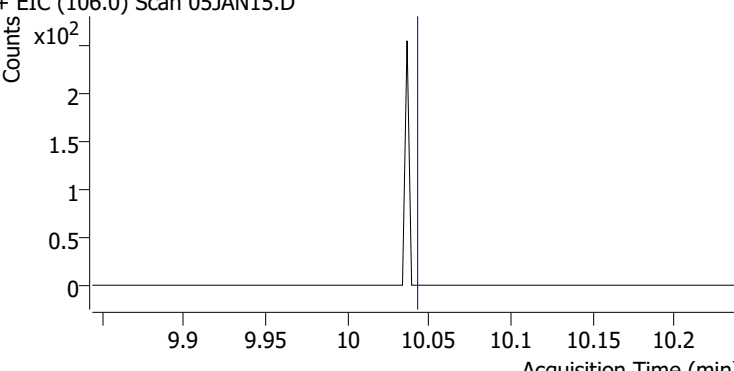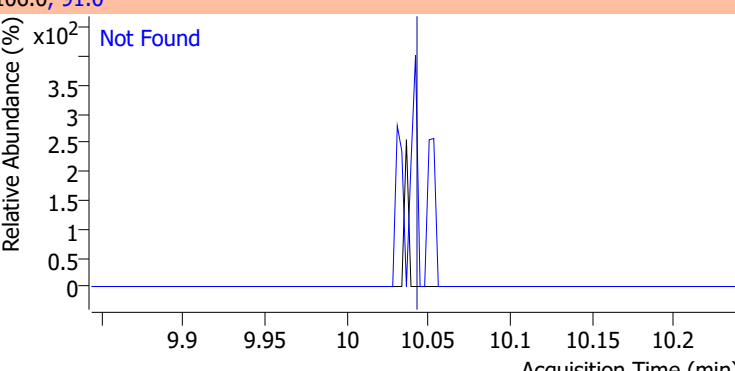
| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--|-------|--------|--|-----------|
| Chlorobenzene | N.D. | 9.80 | 114.0 | 32.1 |
| + EIC (112.0) Scan 05JAN15.D | | | 112.0, 114.0 | |
|  | | |  | |
| 1,1,1,2-Tetrachloroethane | N.D. | 9.89 | 133.0 | 98.6 |
| + EIC (131.0) Scan 05JAN15.D | | | 131.0, 133.0 | |
|  | | |  | |
| Ethylbenzene | N.D. | 9.92 | 106.0 | 31.1 |
| + EIC (91.0) Scan 05JAN15.D | | | 91.0, 106.0 | |
|  | | |  | |
| m+p-Xylenes | N.D. | 10.04 | 91.0 | 201.4 |
| + EIC (106.0) Scan 05JAN15.D | | | 106.0, 91.0 | |
|  | | |  | |


Quantitation Results Report (QT Reviewed)



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------|---------|-------|----------|-------|-------|--------|-------|-------|
| Bromoform | 15.3730 | 10.62 | 0.00 | 4407 | 170.5 | 54.8 | 22.1 | 82.1 |
| | | | | | 174.5 | 43.6 | 20.1 | 80.1 |











| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 270.8078 | 10.95 | 0.00 | 222254 | 174.0 | 92.1 | 61.7 | 121.7 |
| | | | | | 176.0 | 88.4 | 60.6 | 120.6 |



Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|------------------------------|-------|--------|--------------------|-----------|-------|-----------|
| Bromobenzene | N.D. | 11.09 | 77.0 | 145.7 | 158.0 | 96.5 |
| + EIC (156.0) Scan 05JAN15.D | | | 156.0, 77.0, 158.0 | | | |
| | | | | | | |
| 1,1,2,2-Tetrachloroethane | N.D. | 11.12 | 85.0 | 66.2 | | |
| + EIC (83.0) Scan 05JAN15.D | | | 83.0, 85.0 | | | |
| | | | | | | |
| 1,2,3-Trichloropropane | N.D. | 11.15 | 112.0 | 63.5 | | |
| + EIC (110.0) Scan 05JAN15.D | | | 110.0, 112.0 | | | |
| | | | | | | |
| 2-Chlorotoluene | N.D. | 11.29 | 91.0 | 282.3 | | |
| + EIC (126.0) Scan 05JAN15.D | | | 126.0, 91.0 | | | |
| | | | | | | |

Quantitation Results Report (QT Reviewed)
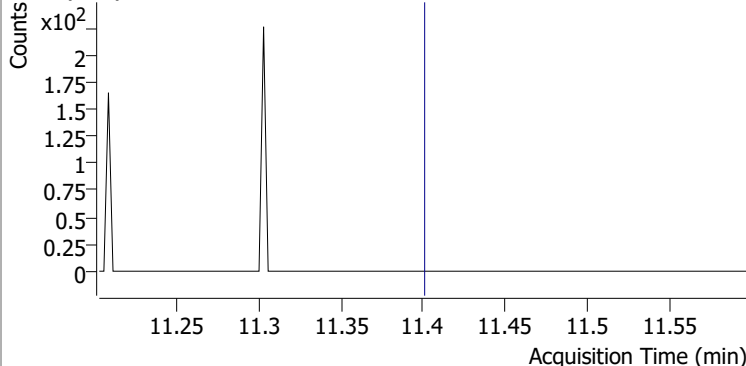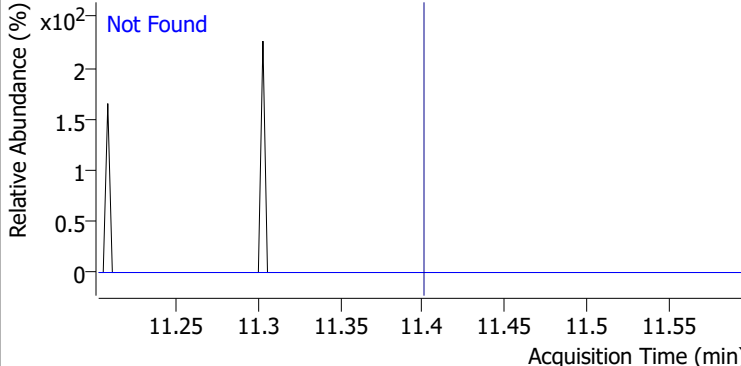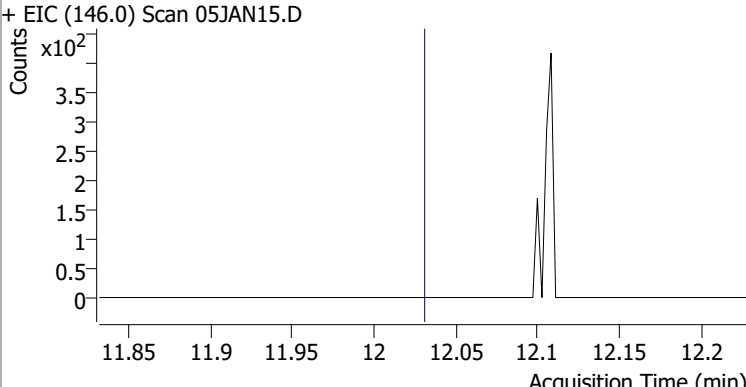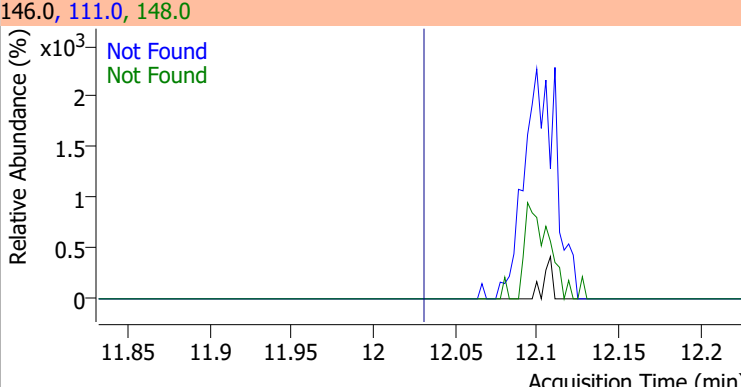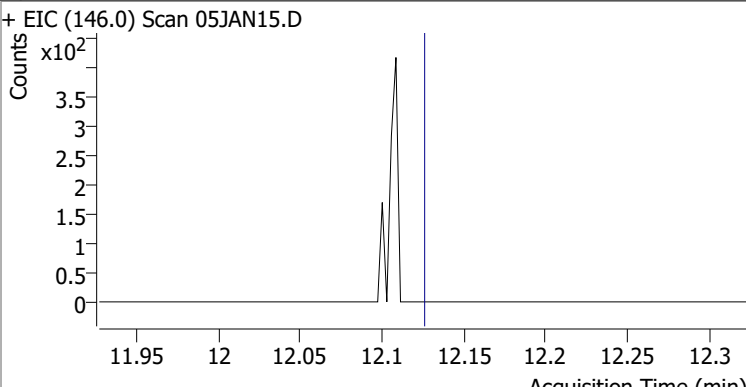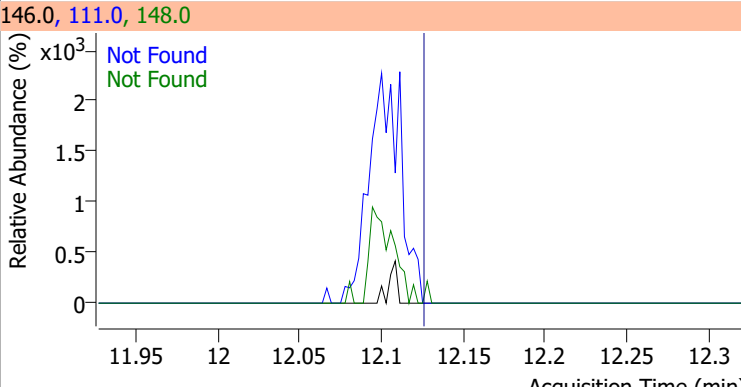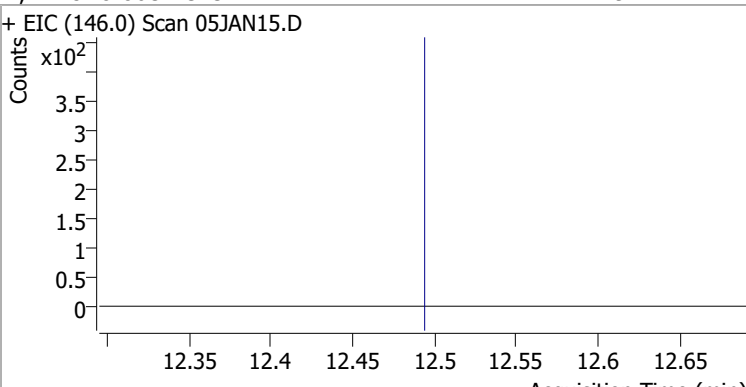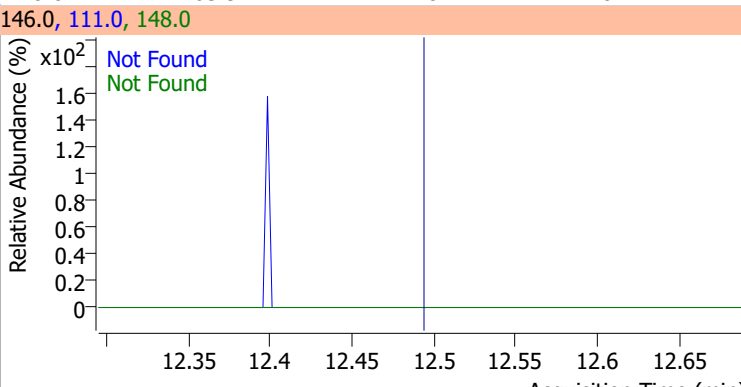
| Compound | Conc. | Exp RT | QIon | Exp Ratio | | |
|--|-------|--------|--|-----------|------|-----------|
| 4-Chlorotoluene | N.D. | 11.40 | 126.0 | 31.7 | | |
| + EIC (91.0) Scan 05JAN15.D | | | 91.0, 126.0 | | | |
|  | | |  | | | |
| 1,3-Dichlorobenzene | N.D. | 12.03 | 148.0 | 63.6 | QIon | Exp Ratio |
| + EIC (146.0) Scan 05JAN15.D | | | 146.0, 111.0, 148.0 | | | |
|  | | |  | | | |
| 1,4-Dichlorobenzene | N.D. | 12.13 | 148.0 | 63.1 | QIon | Exp Ratio |
| + EIC (146.0) Scan 05JAN15.D | | | 146.0, 111.0, 148.0 | | | |
|  | | |  | | | |
| 1,2-Dichlorobenzene | N.D. | 12.49 | 148.0 | 63.9 | QIon | Exp Ratio |
| + EIC (146.0) Scan 05JAN15.D | | | 146.0, 111.0, 148.0 | | | |
|  | | |  | | | |

Quantitation Results Report (QT Reviewed)

| | | | |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File | 05JAN16.D | Operator | MSC |
| Acq. Method | 5975CACQF.M | Acq. Date-Time | 1/5/2022 4:55:12 PM |
| Sample Name | B22010002-003C | Instrument | VOA5975C |
| Vial | 16 | Multiplier | 1.00 |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m | Comment | |
| Tune File | BFB_Atune3.u | Tune Date | 10/11/2021 4:02:00 PM |
| Batch Name | VG010522_8260B.batch.bin | Last Calib Update | 2/28/2022 2:48:47 PM |
| Ref Library | \\MASSHUNTER\Org\Library\NIST129K.l | | |



| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|--------------------|-------|----------|
| Internal Standards | | | | | | |
| M Fluorobenzene | 6.620 | 96.0 | 721651 | 250.0000 | ng | -0.003 |
| M Chlorobenzene-d5 | 9.774 | 82.0 | 281607 | 250.0000 | ng | 0.003 |
| M 1,4-Dichlorobenzene-d4 | 12.100 | 152.0 | 221070 | 250.0000 | ng | 0.000 |
| System Monitoring Compounds | | | | | | |
| S Dibromofluoromethane | 5.845 | 113.0 | 188096 | 276.6653 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 80.0 - 119.0% | | | Recovery = 110.67% | | |
| S 1,2-Dichloroethane-d4 | 6.236 | 67.0 | 83583 | 284.6308 | ng | 0.003 |
| Spiked Amount: 250.000 | Range: 81.0 - 118.0% | | | Recovery = 113.85% | | |
| S Toluene-d8 | 8.319 | 98.0 | 720822 | 265.6225 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 89.0 - 112.0% | | | Recovery = 106.25% | | |
| S p-Bromofluorobenzene | 10.951 | 95.0 | 214236 | 264.5239 | ng | -0.003 |
| Spiked Amount: 250.000 | Range: 85.0 - 114.0% | | | Recovery = 105.81% | | |
| Target Compounds | | | | | | |
| T Dichlorodifluoromethane | 0.000 | | 0 | N.D. | | |
| T Chloromethane | 1.408 | 50.0 | 4649 | 4.0503 | ng | 85 |
| T Vinyl chloride | 0.000 | | 0 | N.D. | | |
| T Bromomethane | 0.000 | | 0 | N.D. | | |
| T Chloroethane | 0.000 | | 0 | N.D. | | |
| T Trichlorofluoromethane | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methylene chloride | 3.330 | 49.0 | 0 | | ng | md 1 |
| T trans-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methyl tert-butyl ether (MTBE) | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloroethane | 0.000 | | 0 | N.D. | | |
| T 2,2-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T cis-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methyl ethyl ketone | 0.000 | | 0 | N.D. | | |
| T Bromochloromethane | 0.000 | | 0 | N.D. | | |
| T Chloroform | 5.647 | 83.0 | 2347 | 1.7084 | ng | 83 |


Quantitation Results Report (QT Reviewed)

| Compound | RT | QIon | Resp. | Conc. | Units | | Dev(Min) |
|-----------------------------|--------|-------|-------|---------|-------|----|----------|
| T 1,1,1-Trichloroethane | 0.000 | | 0 | N.D. | | | |
| T Carbon tetrachloride | 0.000 | | 0 | N.D. | | | |
| T 1,1-Dichloropropene | 0.000 | | 0 | N.D. | | | |
| T Benzene | 6.286 | 78.0 | 421 | 0.1466 | ng | m | 65 |
| T 1,2-Dichloroethane | 0.000 | | 0 | N.D. | | | |
| T Trichloroethene | 0.000 | | 0 | N.D. | | | |
| T 1,2-Dichloropropane | 0.000 | | 0 | N.D. | | | |
| T Dibromomethane | 0.000 | | 0 | N.D. | | | |
| T Bromodichloromethane | 7.585 | 83.0 | 1814 | 2.0816 | ng | m | 77 |
| T cis-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | | |
| T Toluene | 8.386 | 92.0 | 0 | | ng | md | 1 |
| T trans-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | | |
| T 1,1,2-Trichloroethane | 0.000 | | 0 | N.D. | | | |
| T Tetrachloroethene | 0.000 | | 0 | N.D. | | | |
| T 1,3-Dichloropropane | 0.000 | | 0 | N.D. | | | |
| T Chlorodibromomethane | 9.208 | 129.0 | 3282 | 5.7496 | ng | | 98 |
| T 1,2-Dibromoethane | 0.000 | | 0 | N.D. | | | |
| T Chlorobenzene | 0.000 | | 0 | N.D. | | | |
| T 1,1,1,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | | |
| T Ethylbenzene | 0.000 | | 0 | N.D. | | | |
| T m+p-Xylenes | 10.045 | 106.0 | 646 | 0.4778 | ng | m | 90 |
| T o-Xylene | 10.430 | 106.0 | 1444 | 1.1990 | ng | m | 81 |
| T Styrene | 0.000 | | 0 | N.D. | | | |
| T Bromoform | 10.622 | 172.5 | 4627 | 16.3559 | ng | | 96 |
| T Bromobenzene | 0.000 | | 0 | N.D. | | | |
| T 1,1,2,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | | |
| T 1,2,3-Trichloropropane | 0.000 | | 0 | N.D. | | | |
| T 2-Chlorotoluene | 0.000 | | 0 | N.D. | | | |
| T 4-Chlorotoluene | 0.000 | | 0 | N.D. | | | |
| T 1,3-Dichlorobenzene | 0.000 | | 0 | N.D. | | | |
| T 1,4-Dichlorobenzene | 0.000 | | 0 | N.D. | | | |
| T 1,2-Dichlorobenzene | 0.000 | | 0 | N.D. | | | |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|-------------------------|-------|--------|------|-----------|
| Dichlorodifluoromethane | N.D. | 1.24 | 87.0 | 32.3 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------|--------|------|----------|-------|------|--------|-------|-------|
| Chloromethane | 4.0503 | 1.41 | 0.00 | 4649 | 52.0 | 40.5 | 2.1 | 62.1 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------------|-------|--------|------|-----------|
| Vinyl chloride | N.D. | 1.50 | 64.0 | 29.9 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------|-------|--------|------|-----------|
| Bromomethane | N.D. | 1.80 | 94.0 | 104.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------|-------|--------|------|-----------|
| Chloroethane | N.D. | 1.89 | 66.0 | 30.1 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|------------------------|-------|--------|-------|-----------|
| Trichlorofluoromethane | N.D. | 2.14 | 103.0 | 64.2 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethene | N.D. | 2.70 | 61.0 | 180.3 | 63.0 | 56.7 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|-------|----|----------|-------|------|--------|-------|-------|
| Methylene chloride | | 0 | | 0 | 84.0 | | 36.9 | 96.9 |
| | | | | | 86.0 | | 14.3 | 74.3 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,2-Dichloroethene | N.D. | 3.72 | 61.0 | 153.9 | 98.0 | 65.7 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------------------|-------|--------|------|-----------|
| Methyl tert-butyl ether (MTBE) | N.D. | 3.75 | 57.0 | 24.6 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethane | N.D. | 4.38 | 65.0 | 32.1 | 83.0 | 13.7 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|------|-----------|
| 2,2-Dichloropropane | N.D. | 5.20 | 41.0 | 66.5 | 97.0 | 23.2 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|------------------------|-------|--------|------|-----------|------|-----------|
| cis-1,2-Dichloroethene | N.D. | 5.22 | 61.0 | 167.2 | 98.0 | 67.3 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| Methyl ethyl ketone | N.D. | 5.28 | 72.0 | 21.3 |







| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|
| Bromochloromethane | N.D. | 5.52 | 49.0 | 182.9 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|--------|------|----------|-------|------|--------|-------|-------|
| Chloroform | 1.7084 | 5.65 | -0.01 | 2347 | 85.0 | 79.6 | 36.0 | 96.0 |




Quantitation Results Report (QT Reviewed)

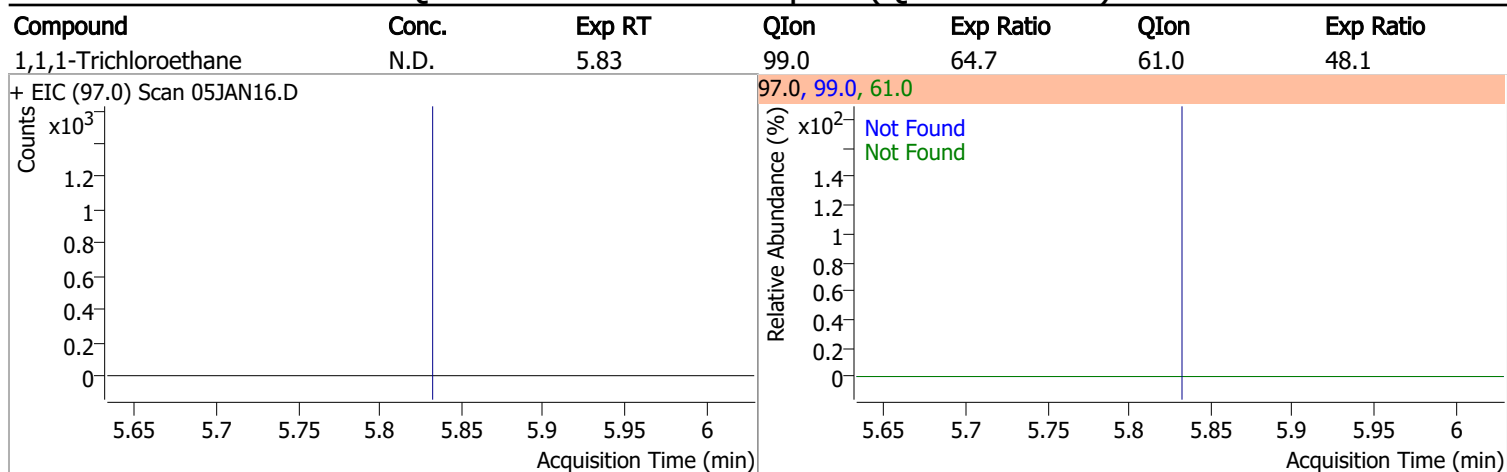


Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 284.6308 | 6.24 | 0.00 | 83583 | 65.0 | 194.1 | 166.5 | 226.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|--------|------|----------|---------|------|--------|-------|-------|
| Benzene | 0.1466 | 6.29 | 0.01 | 421 (m) | 77.0 | 6.6 | 0.0 | 53.5 |







| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,2-Dichloroethane | N.D. | 6.32 | 64.0 | 29.9 | 98.0 | 7.6 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------|-------|--------|-------|-----------|------|-----------|
| Trichloroethene | N.D. | 7.03 | 130.0 | 101.5 | 97.0 | 64.1 |




Quantitation Results Report (QT Reviewed)

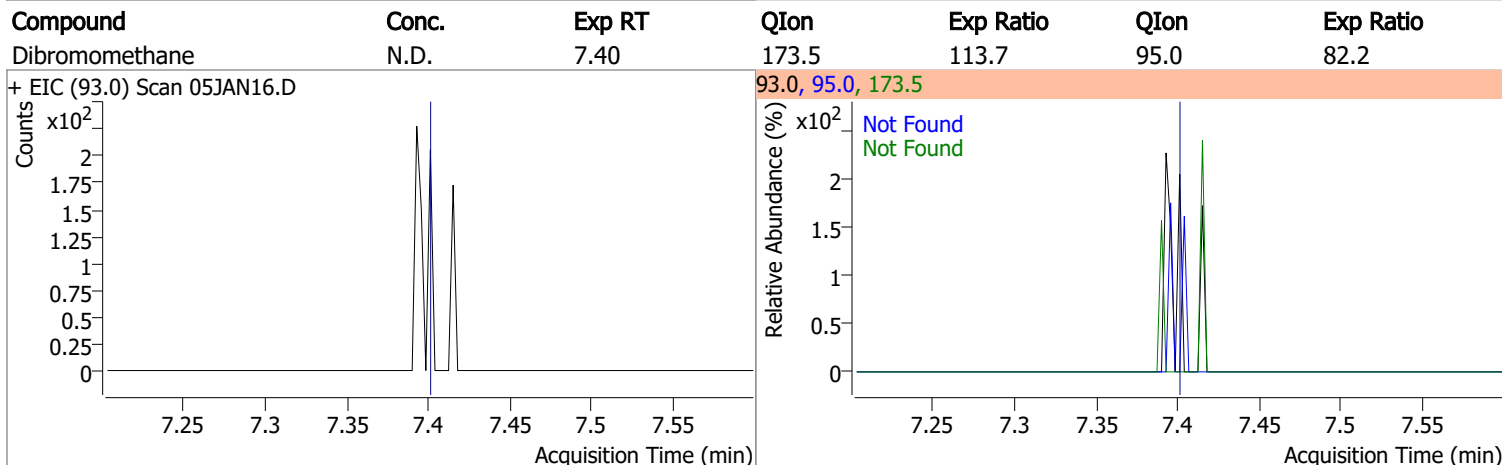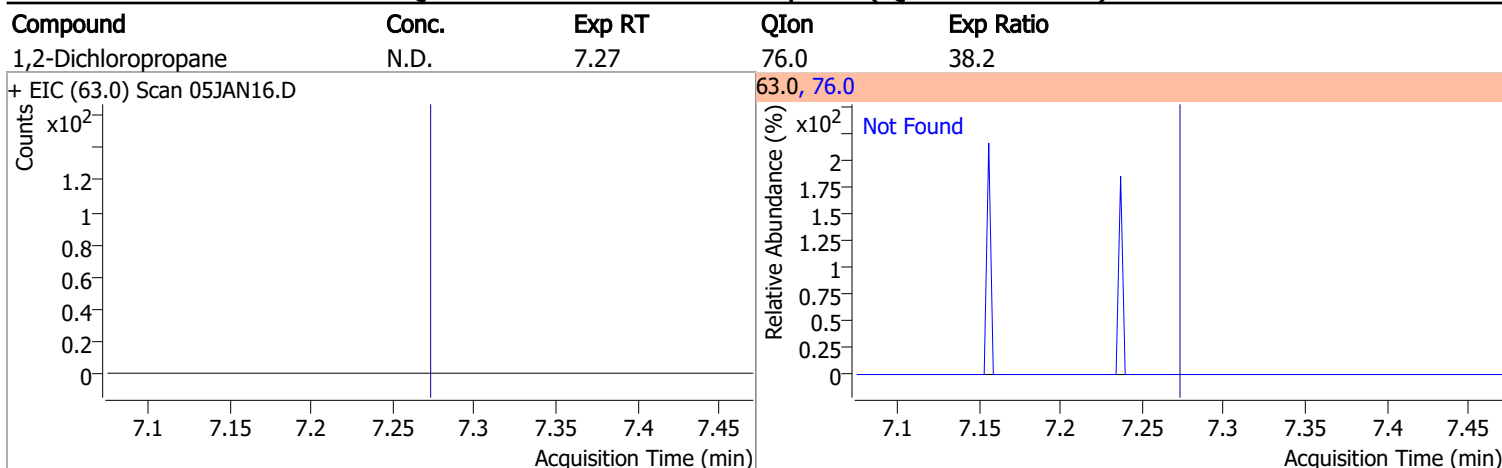


Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 265.6225 | 8.32 | 0.00 | 720822 | 100.0 | 64.7 | 34.4 | 94.4 |
| | | | | | 99.0 | 9.5 | 0.0 | 39.6 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|-------|----|----------|-------|------|--------|-------|-------|
| Toluene | 0 | 0 | 0 | 0 | 91.0 | | 145.8 | 205.8 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,3-Dichloropropene | N.D. | 8.64 | 39.0 | 53.4 | 77.0 | 32.4 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------------|-------|--------|------|-----------|------|-----------|
| 1,1,2-Trichloroethane | N.D. | 8.82 | 97.0 | 114.6 | 85.0 | 67.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-------------------|-------|--------|-------|-----------|-------|-----------|
| Tetrachloroethene | N.D. | 8.94 | 165.8 | 128.6 | 129.0 | 91.5 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| 1,3-Dichloropropane | N.D. | 8.98 | 78.0 | 32.9 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|--------|------|----------|-------|-------|--------|-------|-------|
| Chlorodibromomethane | 5.7496 | 9.21 | 0.00 | 3282 | 127.0 | 76.6 | 48.0 | 108.0 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|-------------------|-------|--------|-------|-----------|
| 1,2-Dibromoethane | N.D. | 9.31 | 109.0 | 94.5 |







Quantitation Results Report (QT Reviewed)









| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|------------------------------|-------|--------------|-------|-----------|
| Chlorobenzene | N.D. | 9.80 | 114.0 | 32.1 |
| + EIC (112.0) Scan 05JAN16.D | | 112.0, 114.0 | | |
| | | | | |
| 1,1,1,2-Tetrachloroethane | N.D. | 9.89 | 133.0 | 98.6 |
| + EIC (131.0) Scan 05JAN16.D | | 131.0, 133.0 | | |
| | | | | |
| Ethylbenzene | N.D. | 9.92 | 106.0 | 31.1 |
| + EIC (91.0) Scan 05JAN16.D | | 91.0, 106.0 | | |
| | | | | |

| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------------|--------|-------------|----------|---------|--|--------|-------|-------|
| m+p-Xylenes | 0.4778 | 10.04 | 0.01 | 646 (m) | 91.0 | 185.6 | 171.4 | 231.4 |
| + EIC (106.0) Scan 05JAN16.D | | 106.0, 91.0 | | | Ratio = 185.6 (92.2 %) Coelution Score | | | |
| | | | | | | | | |









Quantitation Results Report (QT Reviewed)



Quantitation Results Report (QT Reviewed)

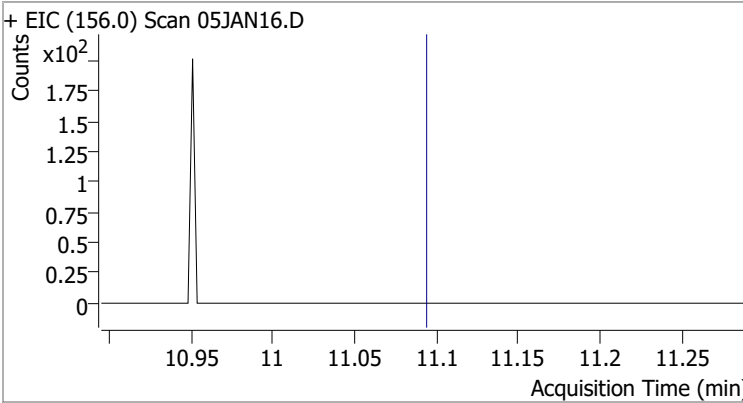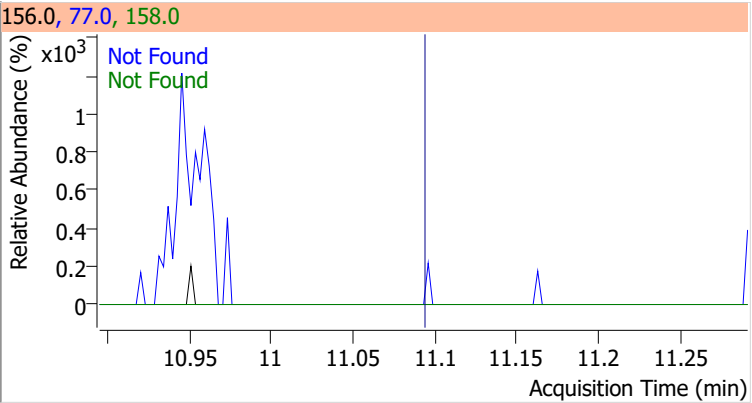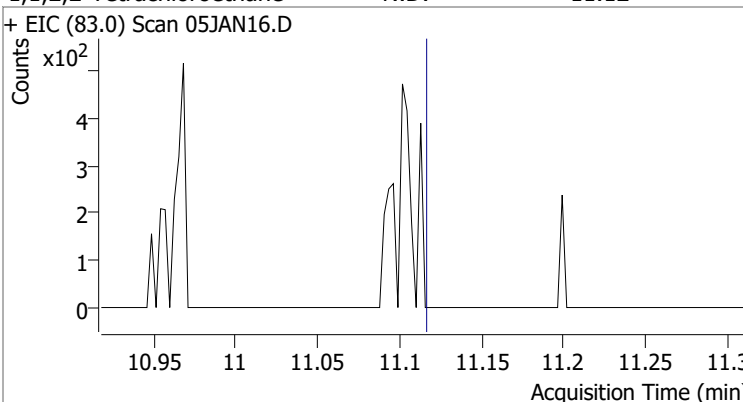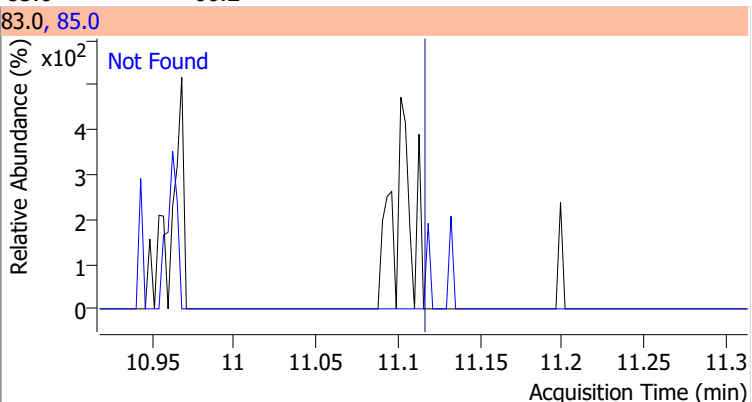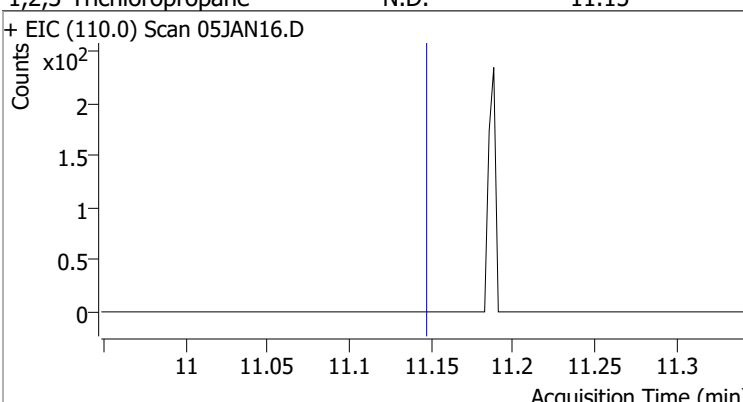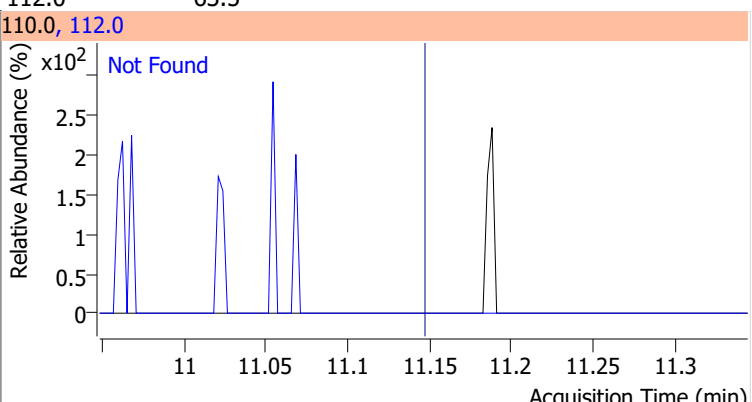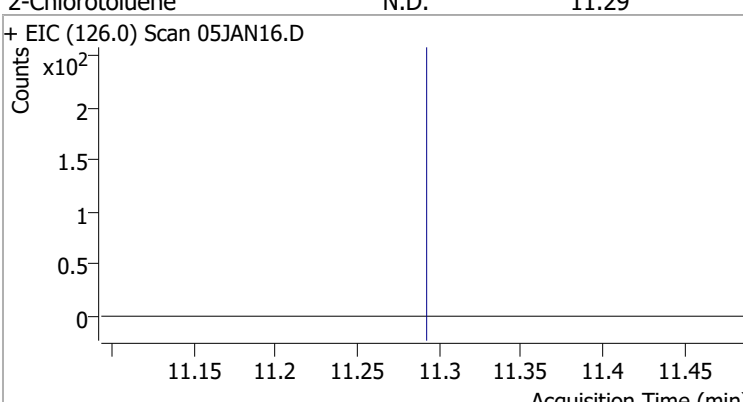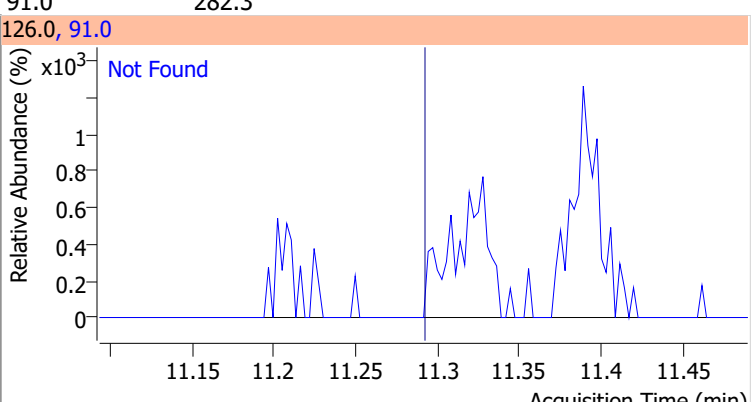
| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--|-------|--------|--|-----------|-------|-----------|
| Bromobenzene | N.D. | 11.09 | 77.0 | 145.7 | 158.0 | 96.5 |
| + EIC (156.0) Scan 05JAN16.D | | | 156.0, 77.0, 158.0 | | | |
|  | | |  | | | |
| 1,1,2,2-Tetrachloroethane | N.D. | 11.12 | 85.0 | 66.2 | | |
| + EIC (83.0) Scan 05JAN16.D | | | 83.0, 85.0 | | | |
|  | | |  | | | |
| 1,2,3-Trichloropropane | N.D. | 11.15 | 112.0 | 63.5 | | |
| + EIC (110.0) Scan 05JAN16.D | | | 110.0, 112.0 | | | |
|  | | |  | | | |
| 2-Chlorotoluene | N.D. | 11.29 | 91.0 | 282.3 | | |
| + EIC (126.0) Scan 05JAN16.D | | | 126.0, 91.0 | | | |
|  | | |  | | | |

Quantitation Results Report (QT Reviewed)
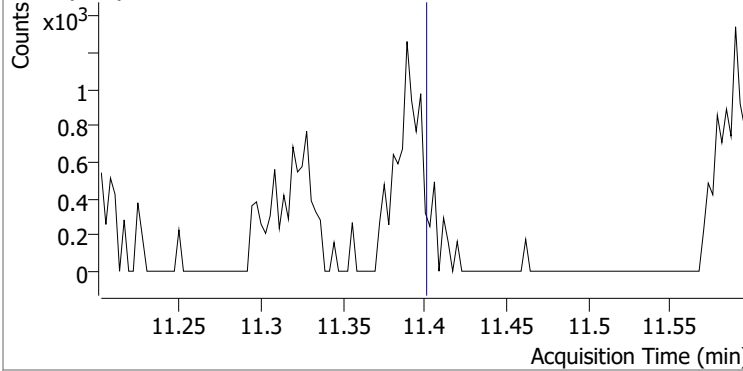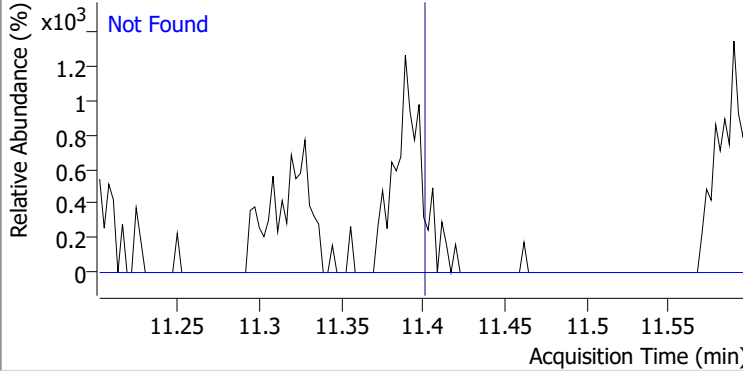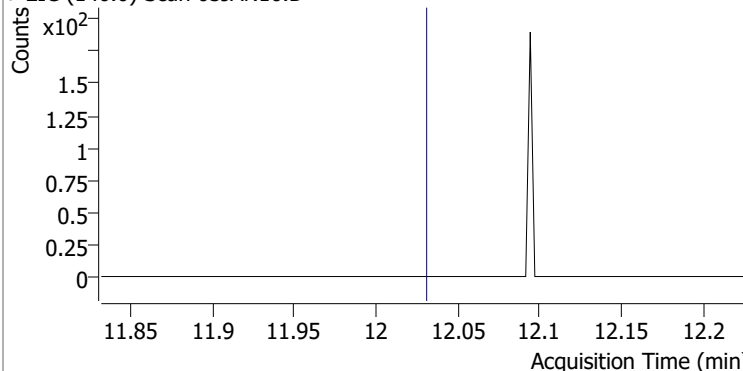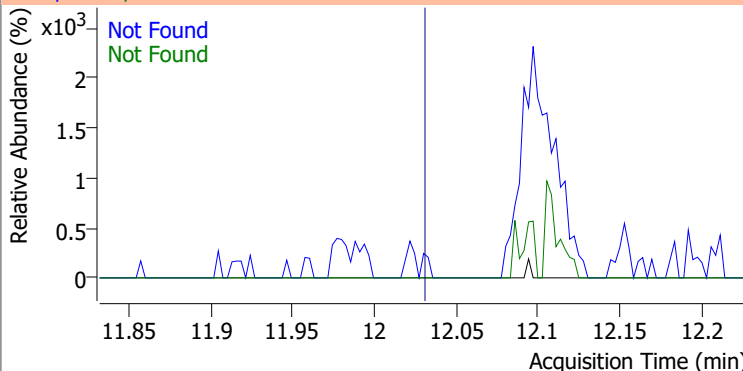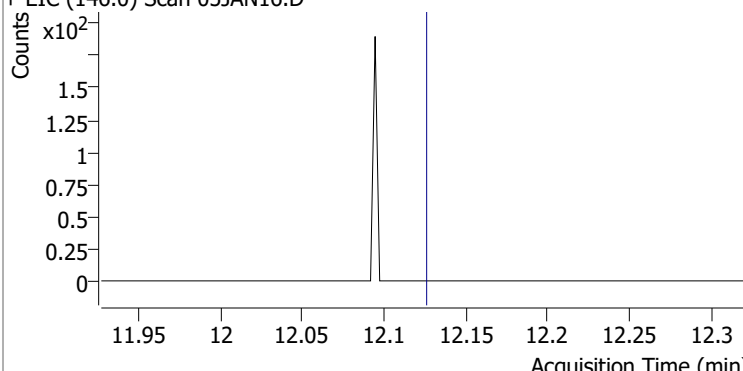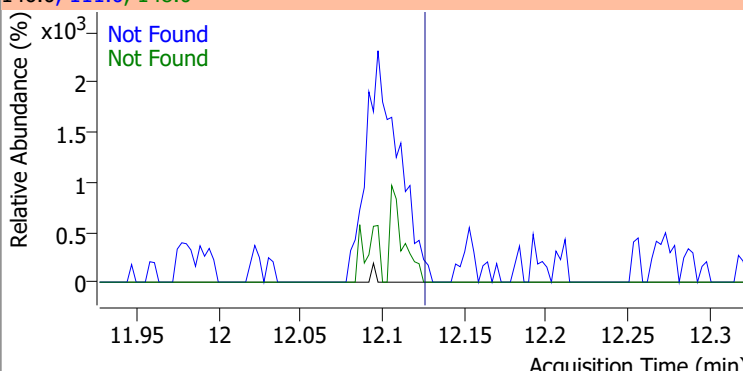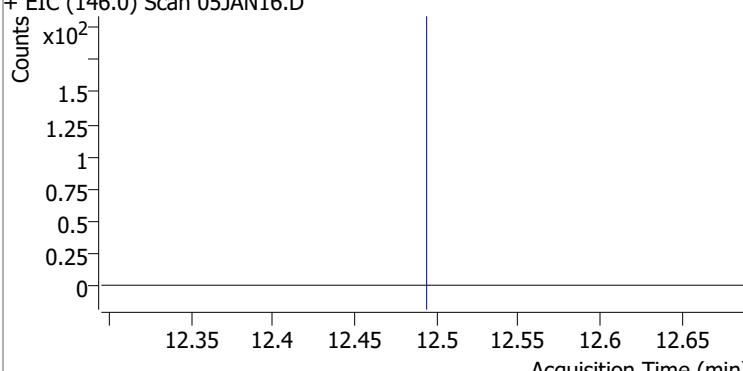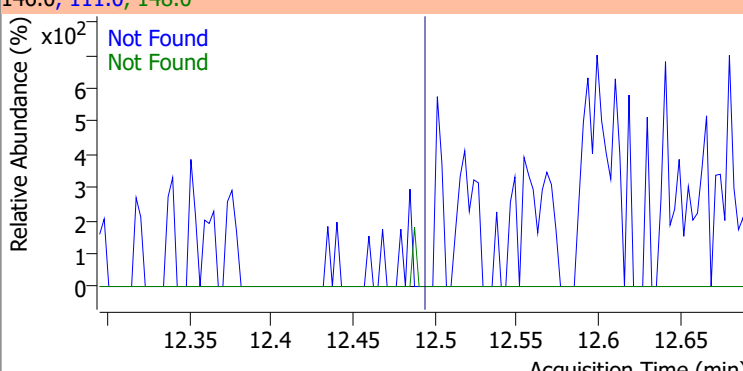
| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--|-------|--------|--|-----------|-------------|-----------|
| 4-Chlorotoluene | N.D. | 11.40 | 126.0 | 31.7 | 91.0, 126.0 | |
| + EIC (91.0) Scan 05JAN16.D  | | |  | | | |
| 1,3-Dichlorobenzene | N.D. | 12.03 | 148.0 | 63.6 | 111.0 | 39.8 |
| + EIC (146.0) Scan 05JAN16.D  | | |  | | | |
| 1,4-Dichlorobenzene | N.D. | 12.13 | 148.0 | 63.1 | 111.0 | 39.1 |
| + EIC (146.0) Scan 05JAN16.D  | | |  | | | |
| 1,2-Dichlorobenzene | N.D. | 12.49 | 148.0 | 63.9 | 111.0 | 41.0 |
| + EIC (146.0) Scan 05JAN16.D  | | |  | | | |

Quantitation Results Report (QT Reviewed)

| | | | |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File | 05JAN17.D | Operator | MSC |
| Acq. Method | 5975CACQF.M | Acq. Date-Time | 1/5/2022 5:22:23 PM |
| Sample Name | B22010096-001F | Instrument | VOA5975C |
| Vial | 17 | Multiplier | 1.00 |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m | Comment | |
| Tune File | BFB_Atune3.u | Tune Date | 10/11/2021 4:02:00 PM |
| Batch Name | VG010522_8260B.batch.bin | Last Calib Update | 2/28/2022 2:48:47 PM |
| Ref Library | \\MASSHUNTER\Org\Library\NIST129K.I | | |



| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|----------|----|------|-------|-------|-------|----------|
|----------|----|------|-------|-------|-------|----------|

Internal Standards

| | | | | | | |
|--------------------------|--------|-------|--------|----------|----|--------|
| M Fluorobenzene | 6.620 | 96.0 | 750361 | 250.0000 | ng | -0.003 |
| M Chlorobenzene-d5 | 9.772 | 82.0 | 288856 | 250.0000 | ng | 0.000 |
| M 1,4-Dichlorobenzene-d4 | 12.100 | 152.0 | 219694 | 250.0000 | ng | 0.000 |

System Monitoring Compounds

| | | | | | | |
|-------------------------|----------------------|-------|--------|--------------------|----|--------|
| S Dibromofluoromethane | 5.848 | 113.0 | 196559 | 278.0514 | ng | 0.003 |
| Spiked Amount: 250.000 | Range: 80.0 - 119.0% | | | Recovery = 111.22% | | |
| S 1,2-Dichloroethane-d4 | 6.233 | 67.0 | 87846 | 287.7020 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 81.0 - 118.0% | | | Recovery = 115.08% | | |
| S Toluene-d8 | 8.319 | 98.0 | 754001 | 270.8761 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 89.0 - 112.0% | | | Recovery = 108.35% | | |
| S p-Bromofluorobenzene | 10.951 | 95.0 | 219103 | 272.2278 | ng | -0.003 |
| Spiked Amount: 250.000 | Range: 85.0 - 114.0% | | | Recovery = 108.89% | | |

Target Compounds

| Compound | RT | QIon | Resp. | Conc. | Units | QValue |
|----------------------------------|-------|------|-------|--------|-------|--------|
| T Dichlorodifluoromethane | 0.000 | | 0 | N.D. | | |
| T Chloromethane | 1.411 | 50.0 | 1055 | 0.8837 | ng m | 81 |
| T Vinyl chloride | 0.000 | | 0 | N.D. | | |
| T Bromomethane | 0.000 | | 0 | N.D. | | |
| T Chloroethane | 0.000 | | 0 | N.D. | | |
| T Trichlorofluoromethane | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methylene chloride | 3.333 | 49.0 | 0 | | ng md | 1 |
| T trans-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methyl tert-butyl ether (MTBE) | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloroethane | 0.000 | | 0 | N.D. | | |
| T 2,2-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T cis-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methyl ethyl ketone | 0.000 | | 0 | N.D. | | |
| T Bromochloromethane | 0.000 | | 0 | N.D. | | |
| T Chloroform | 0.000 | | 0 | N.D. | | |


Quantitation Results Report (QT Reviewed)

| Compound | RT | QIon | Resp. | Conc. | Units | | Dev(Min) |
|-----------------------------|--------|-------|-------|--------|-------|----|----------|
| T 1,1,1-Trichloroethane | 0.000 | | 0 | N.D. | | | |
| T Carbon tetrachloride | 0.000 | | 0 | N.D. | | | |
| T 1,1-Dichloropropene | 0.000 | | 0 | N.D. | | | |
| T Benzene | 0.000 | | 0 | N.D. | | | |
| T 1,2-Dichloroethane | 0.000 | | 0 | N.D. | | | |
| T Trichloroethene | 0.000 | | 0 | N.D. | | | |
| T 1,2-Dichloropropane | 0.000 | | 0 | N.D. | | | |
| T Dibromomethane | 0.000 | | 0 | N.D. | | | |
| T Bromodichloromethane | 0.000 | | 0 | N.D. | | | |
| T cis-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | | |
| T Toluene | 0.000 | | 0 | N.D. | | | |
| T trans-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | | |
| T 1,1,2-Trichloroethane | 0.000 | | 0 | N.D. | | | |
| T Tetrachloroethene | 0.000 | | 0 | N.D. | | | |
| T 1,3-Dichloropropane | 0.000 | | 0 | N.D. | | | |
| T Chlorodibromomethane | 0.000 | | 0 | N.D. | | | |
| T 1,2-Dibromoethane | 0.000 | | 0 | N.D. | | | |
| T Chlorobenzene | 0.000 | | 0 | N.D. | | | |
| T 1,1,1,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | | |
| T Ethylbenzene | 9.914 | 91.0 | 0 | | ng | md | 1 |
| T m+p-Xylenes | 10.042 | 106.0 | 64 | 0.0463 | ng | m | 99 |
| T o-Xylene | 0.000 | | 0 | N.D. | | | |
| T Styrene | 0.000 | | 0 | N.D. | | | |
| T Bromoform | 0.000 | | 0 | N.D. | | | |
| T Bromobenzene | 0.000 | | 0 | N.D. | | | |
| T 1,1,2,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | | |
| T 1,2,3-Trichloropropane | 0.000 | | 0 | N.D. | | | |
| T 2-Chlorotoluene | 0.000 | | 0 | N.D. | | | |
| T 4-Chlorotoluene | 0.000 | | 0 | N.D. | | | |
| T 1,3-Dichlorobenzene | 0.000 | | 0 | N.D. | | | |
| T 1,4-Dichlorobenzene | 0.000 | | 0 | N.D. | | | |
| T 1,2-Dichlorobenzene | 0.000 | | 0 | N.D. | | | |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|-------------------------|-------|--------|------|-----------|
| Dichlorodifluoromethane | N.D. | 1.24 | 87.0 | 32.3 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------|--------|------|----------|----------|------|--------|-------|-------|
| Chloromethane | 0.8837 | 1.41 | 0.00 | 1055 (m) | 52.0 | 21.6 | 2.1 | 62.1 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------------|-------|--------|------|-----------|
| Vinyl chloride | N.D. | 1.50 | 64.0 | 29.9 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------|-------|--------|------|-----------|
| Bromomethane | N.D. | 1.80 | 94.0 | 104.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------|-------|--------|------|-----------|
| Chloroethane | N.D. | 1.89 | 66.0 | 30.1 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|------------------------|-------|--------|-------|-----------|
| Trichlorofluoromethane | N.D. | 2.14 | 103.0 | 64.2 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethene | N.D. | 2.70 | 61.0 | 180.3 | 63.0 | 56.7 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|-------|----|----------|-------|------|--------|-------|-------|
| Methylene chloride | | 0 | | 0 | 84.0 | | 36.9 | 96.9 |
| | | | | | 86.0 | | 14.3 | 74.3 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,2-Dichloroethene | N.D. | 3.72 | 61.0 | 153.9 | 98.0 | 65.7 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------------------|-------|--------|------|-----------|
| Methyl tert-butyl ether (MTBE) | N.D. | 3.75 | 57.0 | 24.6 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethane | N.D. | 4.38 | 65.0 | 32.1 | 83.0 | 13.7 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|------|-----------|
| 2,2-Dichloropropane | N.D. | 5.20 | 41.0 | 66.5 | 97.0 | 23.2 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|------------------------|-------|--------|------|-----------|------|-----------|
| cis-1,2-Dichloroethene | N.D. | 5.22 | 61.0 | 167.2 | 98.0 | 67.3 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| Methyl ethyl ketone | N.D. | 5.28 | 72.0 | 21.3 |







| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|
| Bromochloromethane | N.D. | 5.52 | 49.0 | 182.9 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|------------|-------|--------|------|-----------|
| Chloroform | N.D. | 5.65 | 85.0 | 66.0 |




Quantitation Results Report (QT Reviewed)

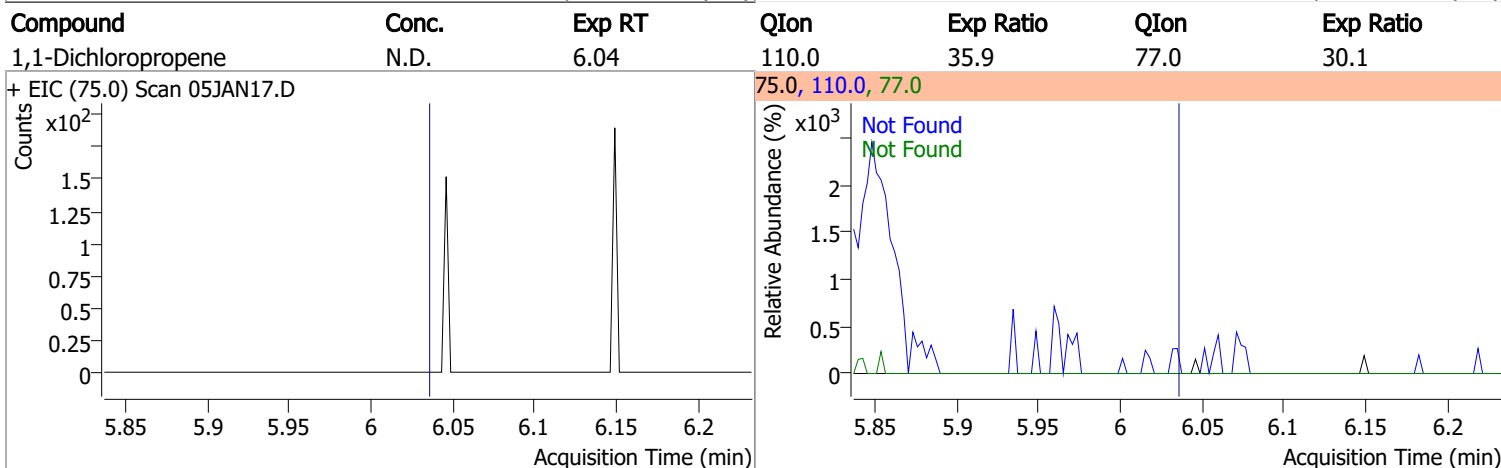


Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 287.7020 | 6.23 | 0.00 | 87846 | 65.0 | 198.4 | 166.5 | 226.5 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------|-------|--------|------|-----------|
| Benzene | N.D. | 6.28 | 77.0 | 23.5 |







| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,2-Dichloroethane | N.D. | 6.32 | 64.0 | 29.9 | 98.0 | 7.6 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------|-------|--------|-------|-----------|------|-----------|
| Trichloroethene | N.D. | 7.03 | 130.0 | 101.5 | 97.0 | 64.1 |




Quantitation Results Report (QT Reviewed)

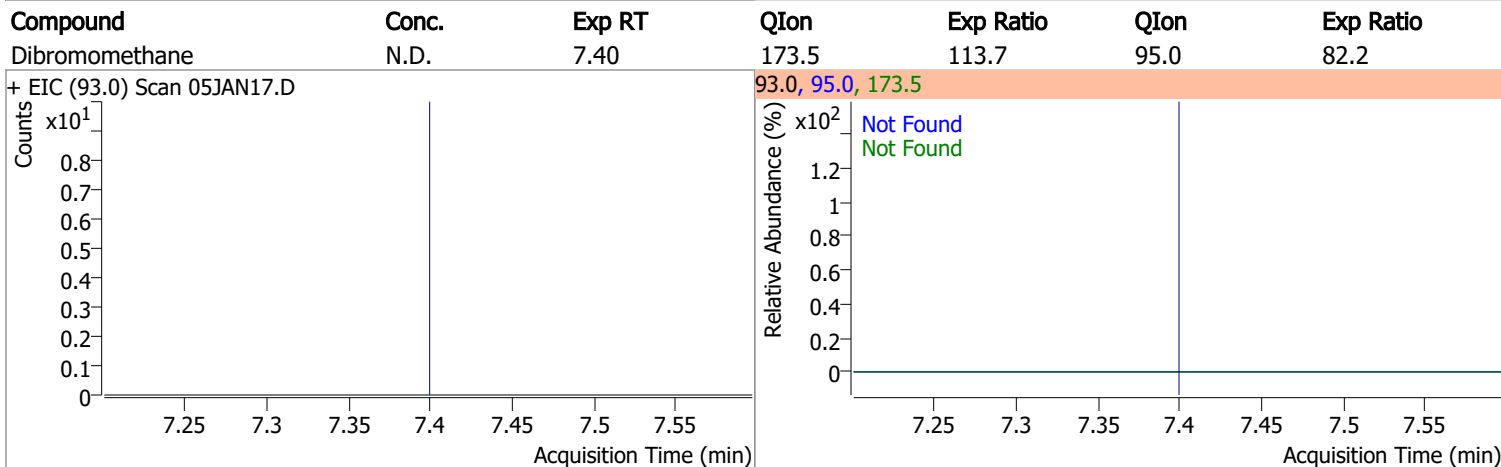


Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 270.8761 | 8.32 | 0.00 | 754001 | 100.0 | 63.5 | 34.4 | 94.4 |
| | | | | | 99.0 | 9.4 | 0.0 | 39.6 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------|-------|--------|------|-----------|
| Toluene | N.D. | 8.39 | 91.0 | 175.8 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,3-Dichloropropene | N.D. | 8.64 | 39.0 | 53.4 | 77.0 | 32.4 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------------|-------|--------|------|-----------|------|-----------|
| 1,1,2-Trichloroethane | N.D. | 8.82 | 97.0 | 114.6 | 85.0 | 67.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-------------------|-------|--------|-------|-----------|-------|-----------|
| Tetrachloroethene | N.D. | 8.94 | 165.8 | 128.6 | 129.0 | 91.5 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| 1,3-Dichloropropane | N.D. | 8.98 | 78.0 | 32.9 |







| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------------------|-------|--------|-------|-----------|
| Chlorodibromomethane | N.D. | 9.21 | 127.0 | 78.0 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|-------------------|-------|--------|-------|-----------|
| 1,2-Dibromoethane | N.D. | 9.31 | 109.0 | 94.5 |




Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------|-------|--------|------|-----------|
| o-Xylene | N.D. | 10.43 | 91.0 | 213.1 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------|-------|--------|------|-----------|
| Styrene | N.D. | 10.45 | 78.0 | 49.6 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------|-------|--------|-------|-----------|-------|-----------|
| Bromoform | N.D. | 10.63 | 170.5 | 52.1 | 174.5 | 50.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 272.2278 | 10.95 | 0.00 | 219103 | 174.0 | 94.5 | 61.7 | 121.7 |
| | | | | | 176.0 | 92.1 | 60.6 | 120.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------|-------|--------|------|-----------|-------|-----------|
| Bromobenzene | N.D. | 11.09 | 77.0 | 145.7 | 158.0 | 96.5 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------------|-------|--------|------|-----------|
| 1,1,2,2-Tetrachloroethane | N.D. | 11.12 | 85.0 | 66.2 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|------------------------|-------|--------|-------|-----------|
| 1,2,3-Trichloropropane | N.D. | 11.15 | 112.0 | 63.5 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|-----------------|-------|--------|------|-----------|
| 2-Chlorotoluene | N.D. | 11.29 | 91.0 | 282.3 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|-----------------|-------|--------|-------|-----------|
| 4-Chlorotoluene | N.D. | 11.40 | 126.0 | 31.7 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|-------|-----------|-------|-----------|
| 1,3-Dichlorobenzene | N.D. | 12.03 | 148.0 | 63.6 | 111.0 | 39.8 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|-------|-----------|-------|-----------|
| 1,4-Dichlorobenzene | N.D. | 12.13 | 148.0 | 63.1 | 111.0 | 39.1 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|-------|-----------|-------|-----------|
| 1,2-Dichlorobenzene | N.D. | 12.49 | 148.0 | 63.9 | 111.0 | 41.0 |



Quantitation Results Report (QT Reviewed)

| | | | |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File | 05JAN18.D | Operator | MSC |
| Acq. Method | 5975CACQF.M | Acq. Date-Time | 1/5/2022 5:49:37 PM |
| Sample Name | B22010120-001F | Instrument | VOA5975C |
| Vial | 18 | Multiplier | 1.00 |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m | Comment | |
| Tune File | BFB_Atune3.u | Tune Date | 10/11/2021 4:02:00 PM |
| Batch Name | VG010522_8260B.batch.bin | Last Calib Update | 2/28/2022 2:48:47 PM |
| Ref Library | \\MASSHUNTER\Org\Library\NIST129K.I | | |



| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|----------|----|------|-------|-------|-------|----------|
|----------|----|------|-------|-------|-------|----------|

Internal Standards

| | | | | | | |
|--------------------------|--------|-------|--------|----------|----|--------|
| M Fluorobenzene | 6.618 | 96.0 | 706175 | 250.0000 | ng | -0.006 |
| M Chlorobenzene-d5 | 9.772 | 82.0 | 271496 | 250.0000 | ng | 0.000 |
| M 1,4-Dichlorobenzene-d4 | 12.100 | 152.0 | 209807 | 250.0000 | ng | 0.000 |

System Monitoring Compounds

| | | | | | | |
|-------------------------|----------------------|-------|--------|--------------------|----|--------|
| S Dibromofluoromethane | 5.845 | 113.0 | 184693 | 277.6134 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 80.0 - 119.0% | | | Recovery = 111.05% | | |
| S 1,2-Dichloroethane-d4 | 6.233 | 67.0 | 84286 | 293.3150 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 81.0 - 118.0% | | | Recovery = 117.33% | | |
| S Toluene-d8 | 8.321 | 98.0 | 706225 | 269.9354 | ng | 0.003 |
| Spiked Amount: 250.000 | Range: 89.0 - 112.0% | | | Recovery = 107.97% | | |
| S p-Bromofluorobenzene | 10.948 | 95.0 | 205119 | 266.8629 | ng | -0.006 |
| Spiked Amount: 250.000 | Range: 85.0 - 114.0% | | | Recovery = 106.75% | | |

Target Compounds









| Compound | RT | QIon | Resp. | Conc. | Units | QValue |
|----------------------------------|-------|------|-------|--------|-------|--------|
| T Dichlorodifluoromethane | 0.000 | | 0 | N.D. | | |
| T Chloromethane | 0.000 | | 0 | N.D. | | |
| T Vinyl chloride | 0.000 | | 0 | N.D. | | |
| T Bromomethane | 0.000 | | 0 | N.D. | | |
| T Chloroethane | 0.000 | | 0 | N.D. | | |
| T Trichlorofluoromethane | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methylene chloride | 3.341 | 49.0 | 441 | 0.4210 | ng | m 97 |
| T trans-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methyl tert-butyl ether (MTBE) | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloroethane | 0.000 | | 0 | N.D. | | |
| T 2,2-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T cis-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methyl ethyl ketone | 0.000 | | 0 | N.D. | | |
| T Bromochloromethane | 0.000 | | 0 | N.D. | | |
| T Chloroform | 0.000 | | 0 | N.D. | | |

Quantitation Results Report (QT Reviewed)

| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|-----------------------------|--------|-------|-------|--------|-------|----------|
| T 1,1,1-Trichloroethane | 0.000 | | 0 | N.D. | | |
| T Carbon tetrachloride | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloropropene | 0.000 | | 0 | N.D. | | |
| T Benzene | 0.000 | | 0 | N.D. | | |
| T 1,2-Dichloroethane | 6.316 | 62.0 | 4564 | 6.0003 | ng | 96 |
| T Trichloroethene | 0.000 | | 0 | N.D. | | |
| T 1,2-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T Dibromomethane | 0.000 | | 0 | N.D. | | |
| T Bromodichloromethane | 0.000 | | 0 | N.D. | | |
| T cis-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | |
| T Toluene | 0.000 | | 0 | N.D. | | |
| T trans-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | |
| T 1,1,2-Trichloroethane | 0.000 | | 0 | N.D. | | |
| T Tetrachloroethene | 0.000 | | 0 | N.D. | | |
| T 1,3-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T Chlorodibromomethane | 0.000 | | 0 | N.D. | | |
| T 1,2-Dibromoethane | 0.000 | | 0 | N.D. | | |
| T Chlorobenzene | 0.000 | | 0 | N.D. | | |
| T 1,1,1,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | |
| T Ethylbenzene | 0.000 | | 0 | N.D. | | |
| T m+p-Xylenes | 10.045 | 106.0 | 0 | | ng md | 1 |
| T o-Xylene | 0.000 | | 0 | N.D. | | |
| T Styrene | 0.000 | | 0 | N.D. | | |
| T Bromoform | 0.000 | | 0 | N.D. | | |
| T Bromobenzene | 0.000 | | 0 | N.D. | | |
| T 1,1,2,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | |
| T 1,2,3-Trichloropropane | 0.000 | | 0 | N.D. | | |
| T 2-Chlorotoluene | 0.000 | | 0 | N.D. | | |
| T 4-Chlorotoluene | 0.000 | | 0 | N.D. | | |
| T 1,3-Dichlorobenzene | 0.000 | | 0 | N.D. | | |
| T 1,4-Dichlorobenzene | 0.000 | | 0 | N.D. | | |
| T 1,2-Dichlorobenzene | 0.000 | | 0 | N.D. | | |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)

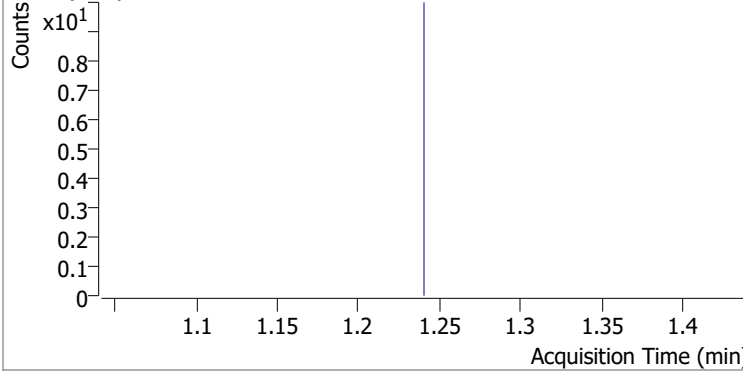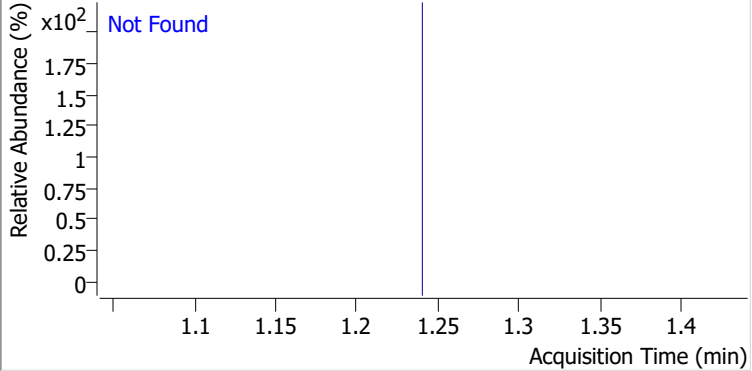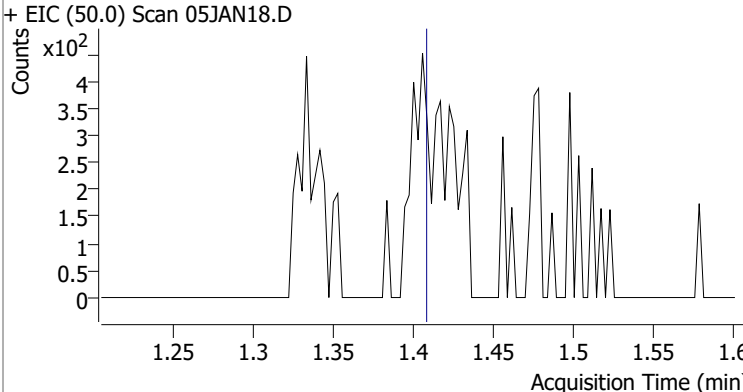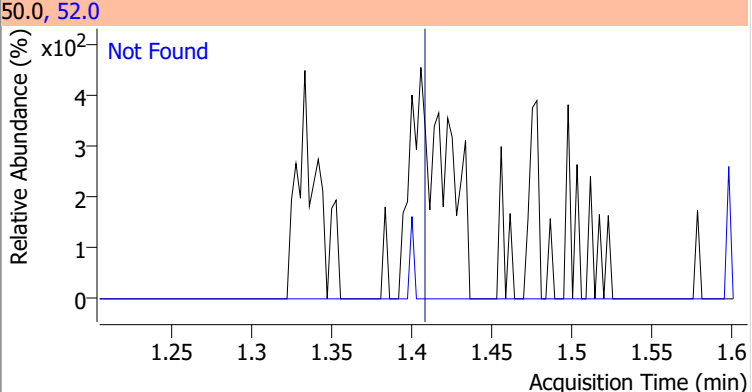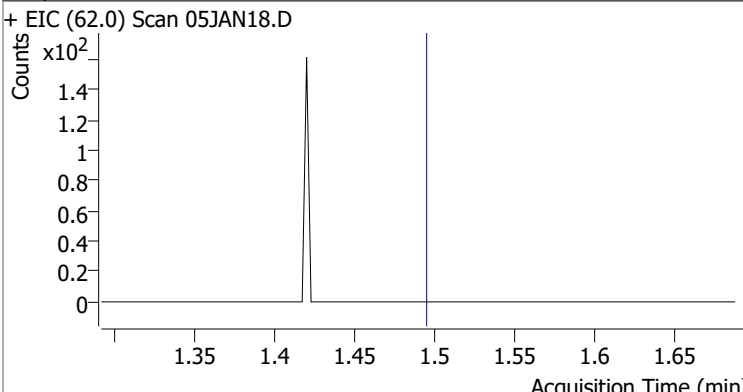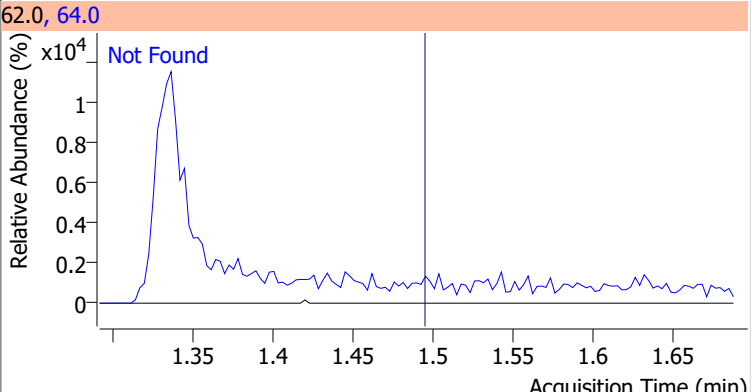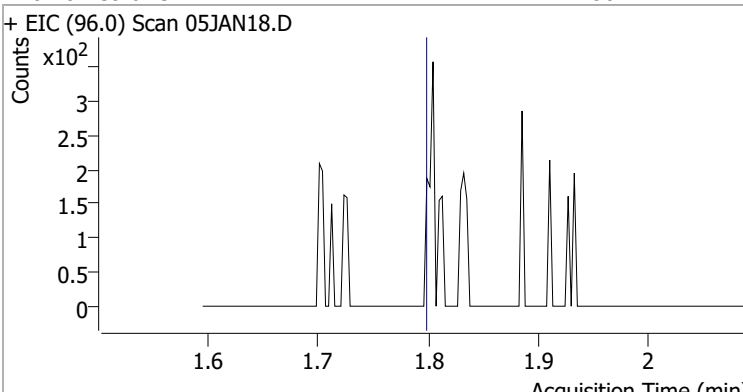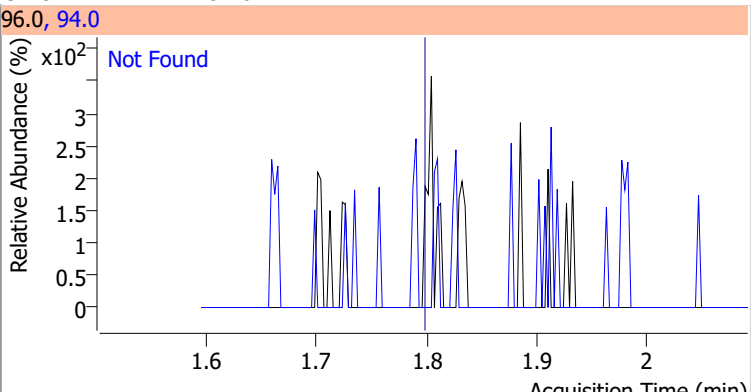
| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--|-------|--------|--|-----------|
| Dichlorodifluoromethane | N.D. | 1.24 | 87.0 | 32.3 |
| + EIC (85.0) Scan 05JAN18.D ***NO DATA POINTS*** | | | 85.0, 87.0 | |
|  | | |  | |
| Chloromethane | N.D. | 1.41 | 52.0 | 32.1 |
| + EIC (50.0) Scan 05JAN18.D | | | 50.0, 52.0 | |
|  | | |  | |
| Vinyl chloride | N.D. | 1.50 | 64.0 | 29.9 |
| + EIC (62.0) Scan 05JAN18.D | | | 62.0, 64.0 | |
|  | | |  | |
| Bromomethane | N.D. | 1.80 | 94.0 | 104.6 |
| + EIC (96.0) Scan 05JAN18.D | | | 96.0, 94.0 | |
|  | | |  | |

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------|-------|--------|------|-----------|
| Chloroethane | N.D. | 1.89 | 66.0 | 30.1 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|------------------------|-------|--------|-------|-----------|
| Trichlorofluoromethane | N.D. | 2.14 | 103.0 | 64.2 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethene | N.D. | 2.70 | 61.0 | 180.3 | 63.0 | 56.7 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|--------|------|----------|---------|------|--------|-------|-------|
| Methylene chloride | 0.4210 | 3.34 | 0.01 | 441 (m) | 84.0 | 67.7 | 36.9 | 96.9 |
| | | | | | 86.0 | 39.7 | 14.3 | 74.3 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,2-Dichloroethene | N.D. | 3.72 | 61.0 | 153.9 | 98.0 | 65.7 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------------------|-------|--------|------|-----------|
| Methyl tert-butyl ether (MTBE) | N.D. | 3.75 | 57.0 | 24.6 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethane | N.D. | 4.38 | 65.0 | 32.1 | 83.0 | 13.7 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|------|-----------|
| 2,2-Dichloropropane | N.D. | 5.20 | 41.0 | 66.5 | 97.0 | 23.2 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|------------------------|-------|--------|------|-----------|------|-----------|
| cis-1,2-Dichloroethene | N.D. | 5.22 | 61.0 | 167.2 | 98.0 | 67.3 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| Methyl ethyl ketone | N.D. | 5.28 | 72.0 | 21.3 |







| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|
| Bromochloromethane | N.D. | 5.52 | 49.0 | 182.9 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|------------|-------|--------|------|-----------|
| Chloroform | N.D. | 5.65 | 85.0 | 66.0 |




Quantitation Results Report (QT Reviewed)

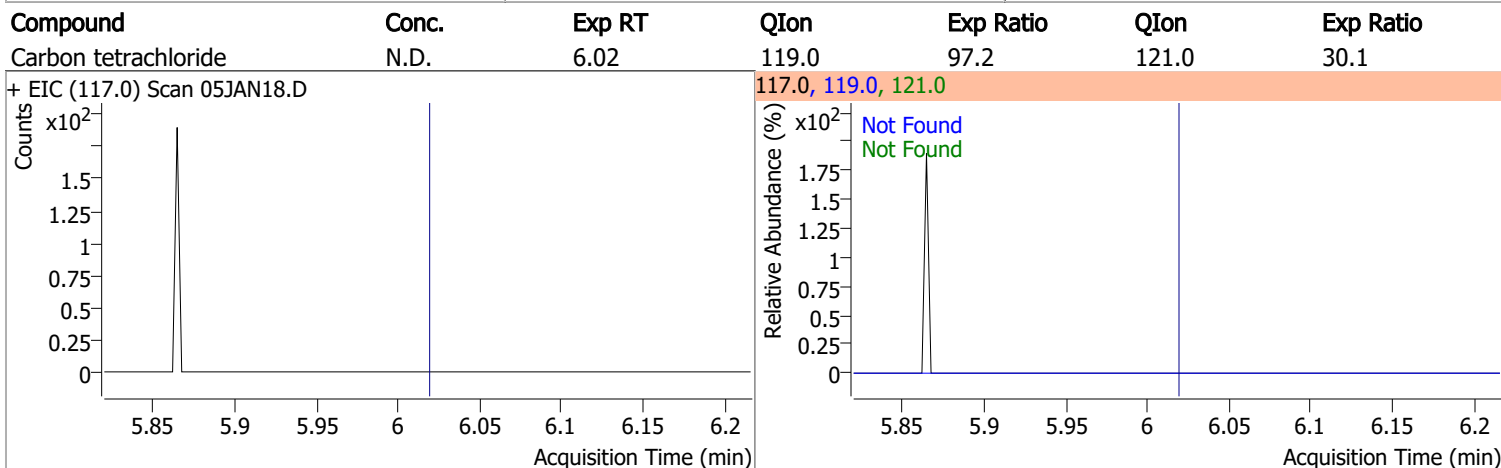


Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 293.3150 | 6.23 | 0.00 | 84286 | 65.0 | 194.7 | 166.5 | 226.5 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------|-------|--------|------|-----------|
| Benzene | N.D. | 6.28 | 77.0 | 23.5 |







| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|--------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane | 6.0003 | 6.32 | -0.01 | 4564 | 64.0 | 31.2 | 0.0 | 59.9 |
| | | | | | 98.0 | 3.3 | 0.0 | 37.6 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------|-------|--------|-------|-----------|------|-----------|
| Trichloroethene | N.D. | 7.03 | 130.0 | 101.5 | 97.0 | 64.1 |




Quantitation Results Report (QT Reviewed)

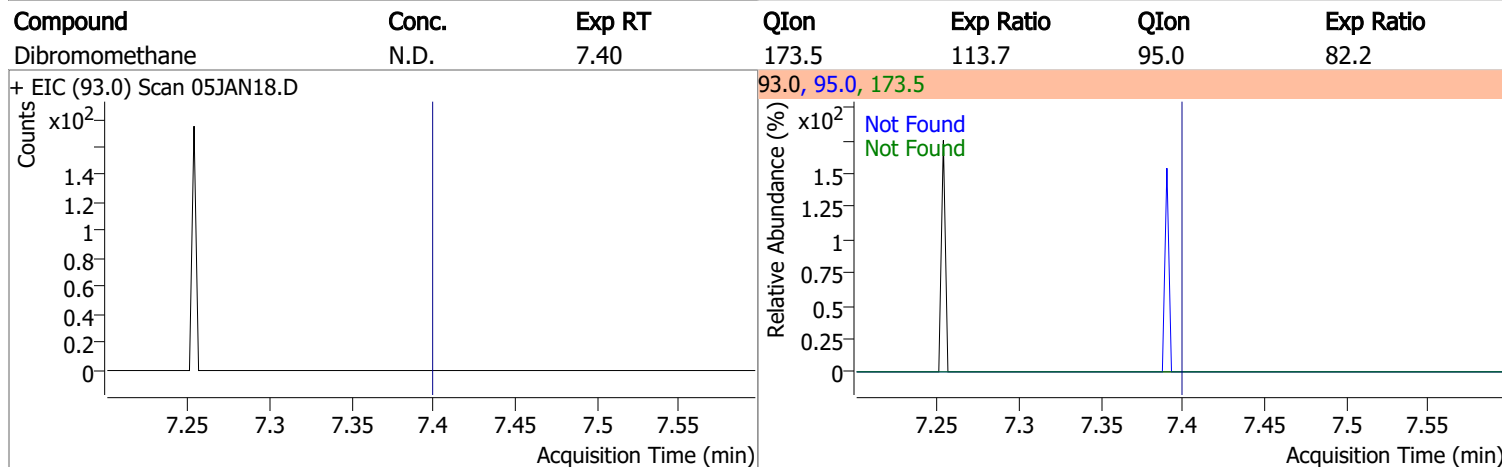


Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 269.9354 | 8.32 | 0.00 | 706225 | 100.0 | 63.8 | 34.4 | 94.4 |
| | | | | | 99.0 | 9.4 | 0.0 | 39.6 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------|-------|--------|------|-----------|
| Toluene | N.D. | 8.39 | 91.0 | 175.8 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,3-Dichloropropene | N.D. | 8.64 | 39.0 | 53.4 | 77.0 | 32.4 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------------|-------|--------|------|-----------|------|-----------|
| 1,1,2-Trichloroethane | N.D. | 8.82 | 97.0 | 114.6 | 85.0 | 67.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-------------------|-------|--------|-------|-----------|-------|-----------|
| Tetrachloroethene | N.D. | 8.94 | 165.8 | 128.6 | 129.0 | 91.5 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| 1,3-Dichloropropane | N.D. | 8.98 | 78.0 | 32.9 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------------------|-------|--------|-------|-----------|
| Chlorodibromomethane | N.D. | 9.21 | 127.0 | 78.0 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|-------------------|-------|--------|-------|-----------|
| 1,2-Dibromoethane | N.D. | 9.31 | 109.0 | 94.5 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------|-------|--------|-------|-----------|
| Chlorobenzene | N.D. | 9.80 | 114.0 | 32.1 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------------|-------|--------|-------|-----------|
| 1,1,1,2-Tetrachloroethane | N.D. | 9.89 | 133.0 | 98.6 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------|-------|--------|-------|-----------|
| Ethylbenzene | N.D. | 9.92 | 106.0 | 31.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------|-------|----|----------|-------|------|--------|-------|-------|
| m+p-Xylenes | | 0 | | 0 | 91.0 | | 171.4 | 231.4 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------|-------|--------|------|-----------|
| o-Xylene | N.D. | 10.43 | 91.0 | 213.1 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------|-------|--------|------|-----------|
| Styrene | N.D. | 10.45 | 78.0 | 49.6 |











| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------|-------|--------|-------|-----------|-------|-----------|
| Bromoform | N.D. | 10.63 | 170.5 | 52.1 | 174.5 | 50.1 |











| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 266.8629 | 10.95 | -0.01 | 205119 | 174.0 | 94.0 | 61.7 | 121.7 |
| | | | | | 176.0 | 90.3 | 60.6 | 120.6 |



Quantitation Results Report (QT Reviewed)

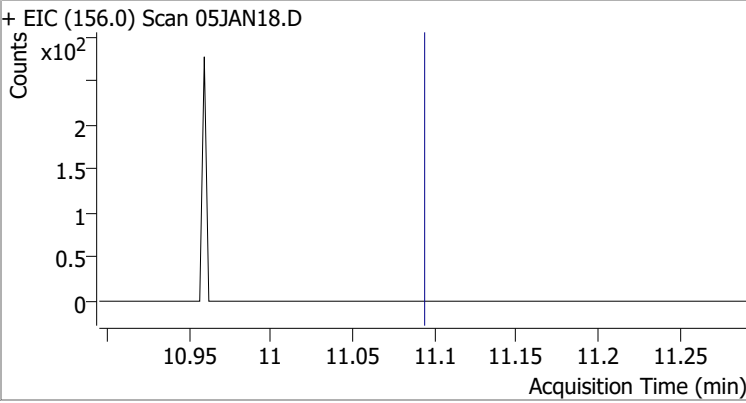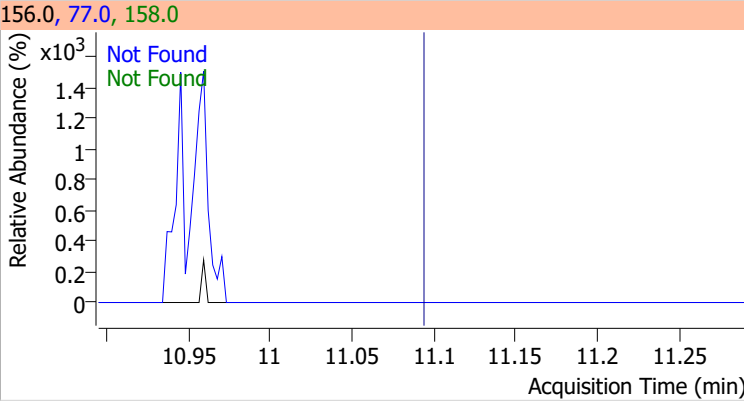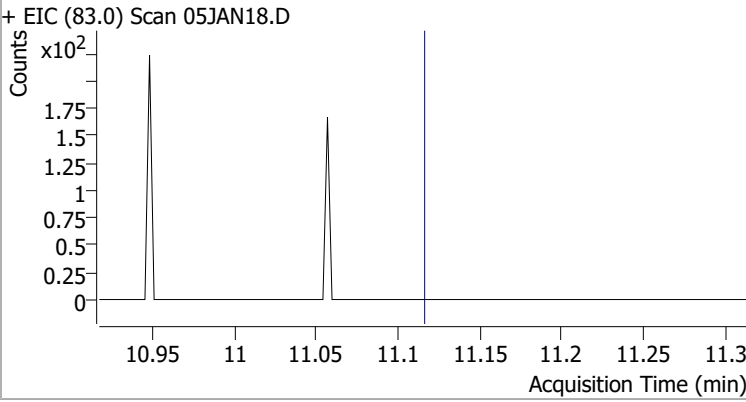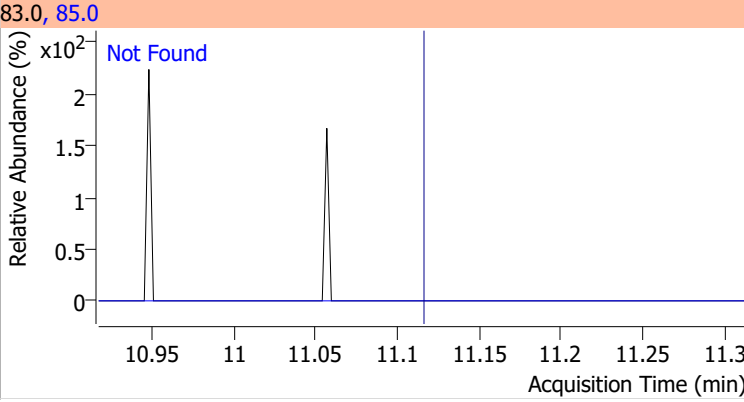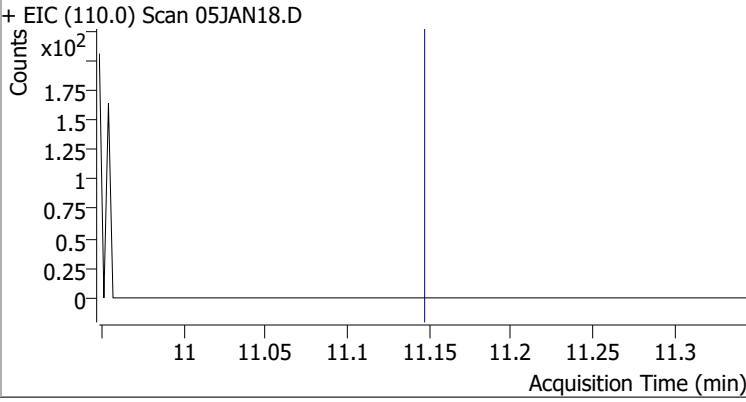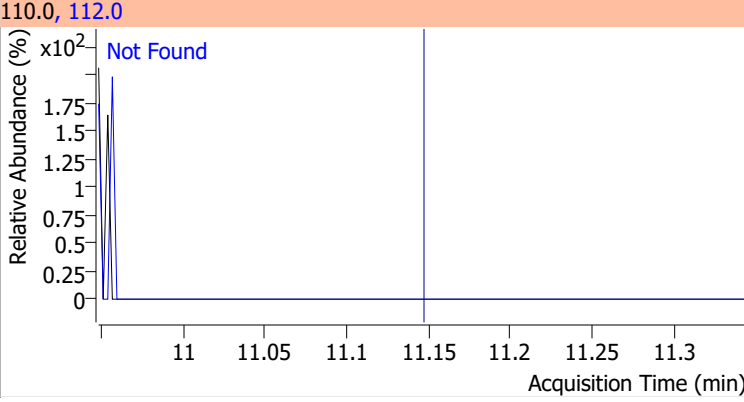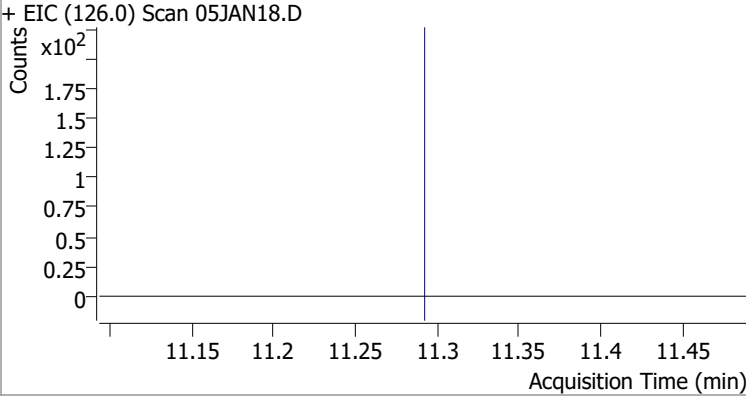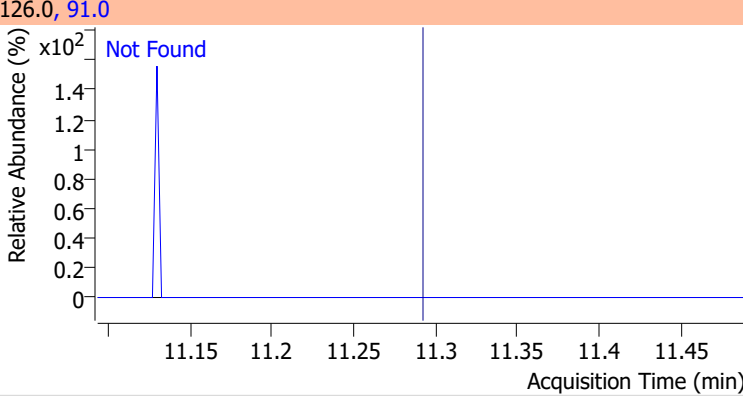
| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--|-------|--------|--|-----------|-------|-----------|
| Bromobenzene | N.D. | 11.09 | 77.0 | 145.7 | 158.0 | 96.5 |
| + EIC (156.0) Scan 05JAN18.D | | | 156.0, 77.0, 158.0 | | | |
|  | | |  | | | |
| 1,1,2,2-Tetrachloroethane | N.D. | 11.12 | 85.0 | 66.2 | | |
| + EIC (83.0) Scan 05JAN18.D | | | 83.0, 85.0 | | | |
|  | | |  | | | |
| 1,2,3-Trichloropropane | N.D. | 11.15 | 112.0 | 63.5 | | |
| + EIC (110.0) Scan 05JAN18.D | | | 110.0, 112.0 | | | |
|  | | |  | | | |
| 2-Chlorotoluene | N.D. | 11.29 | 91.0 | 282.3 | | |
| + EIC (126.0) Scan 05JAN18.D | | | 126.0, 91.0 | | | |
|  | | |  | | | |

Quantitation Results Report (QT Reviewed)
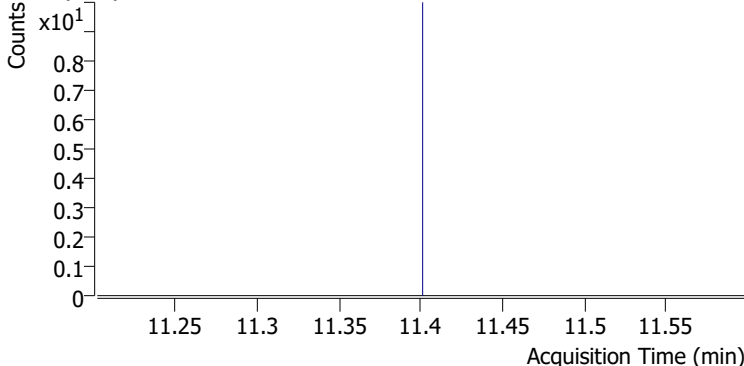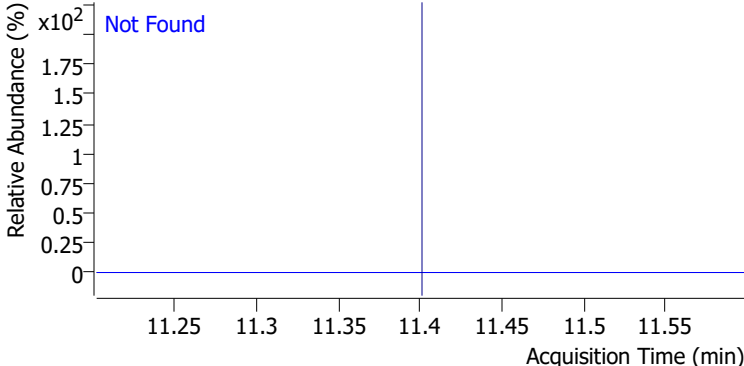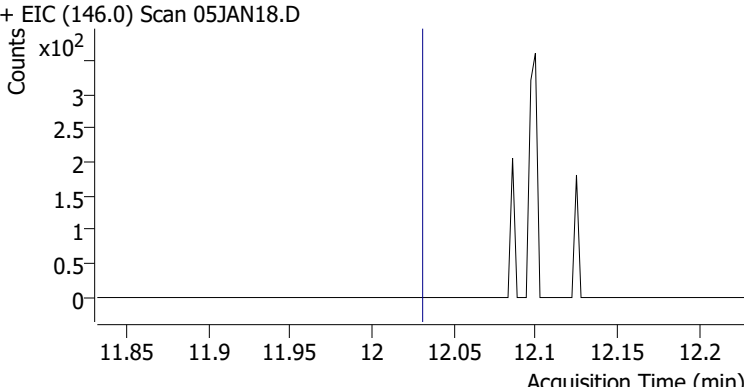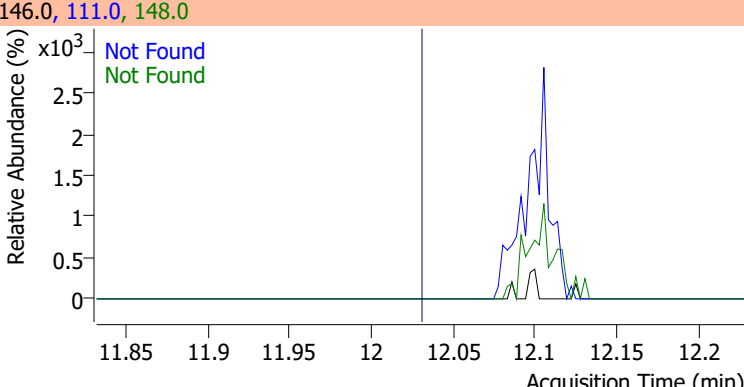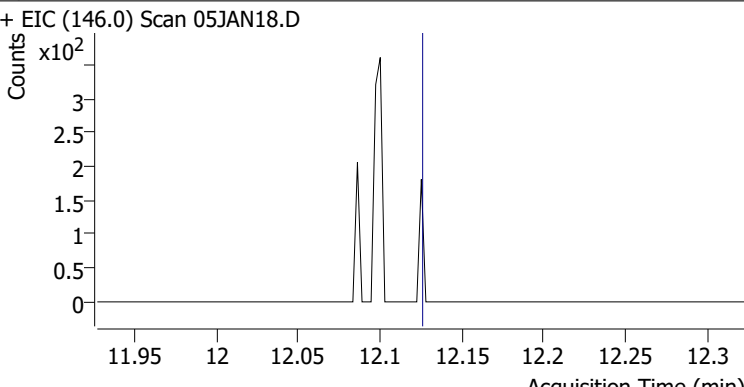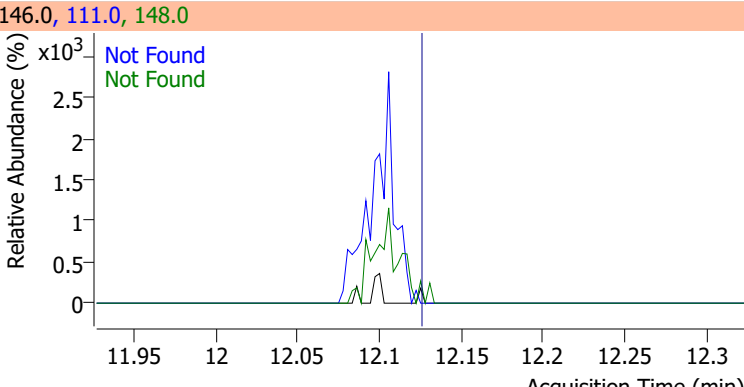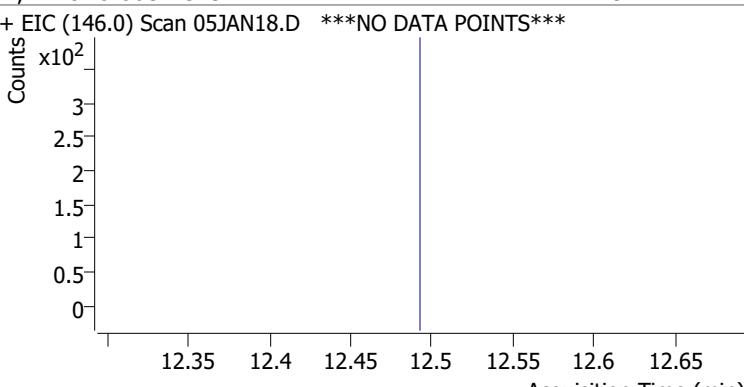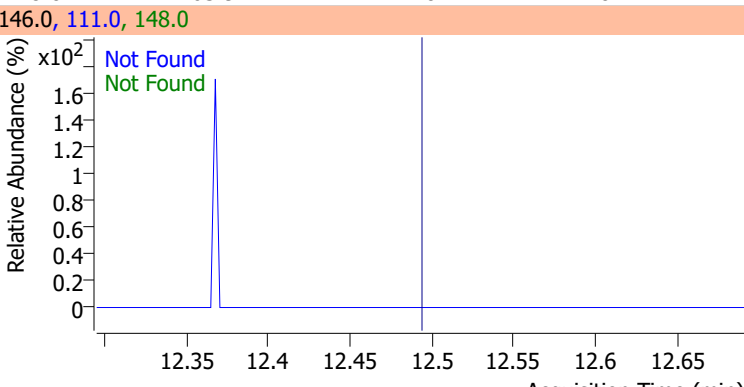
| Compound | Conc. | Exp RT | QIon | Exp Ratio | | | | |
|--|-------|--------|--|-----------|------|-----------|--|--|
| 4-Chlorotoluene | N.D. | 11.40 | 126.0 | 31.7 | | | | |
| + EIC (91.0) Scan 05JAN18.D | | | 91.0, 126.0 | | | | | |
|  | | |  | | | | | |
| 1,3-Dichlorobenzene | N.D. | 12.03 | 148.0 | 63.6 | QIon | Exp Ratio | | |
| + EIC (146.0) Scan 05JAN18.D | | | 146.0, 111.0, 148.0 | | | | | |
|  | | |  | | | | | |
| 1,4-Dichlorobenzene | N.D. | 12.13 | 148.0 | 63.1 | QIon | Exp Ratio | | |
| + EIC (146.0) Scan 05JAN18.D | | | 146.0, 111.0, 148.0 | | | | | |
|  | | |  | | | | | |
| 1,2-Dichlorobenzene | N.D. | 12.49 | 148.0 | 63.9 | QIon | Exp Ratio | | |
| + EIC (146.0) Scan 05JAN18.D ***NO DATA POINTS*** | | | 146.0, 111.0, 148.0 | | | | | |
|  | | |  | | | | | |

Quantitation Results Report (QT Reviewed)

| | | | |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File | 05JAN19.D | Operator | MSC |
| Acq. Method | 5975CACQF.M | Acq. Date-Time | 1/5/2022 6:16:51 PM |
| Sample Name | B22010134-001F | Instrument | VOA5975C |
| Vial | 19 | Multiplier | 1.00 |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m | Comment | |
| Tune File | BFB_Atune3.u | Tune Date | 10/11/2021 4:02:00 PM |
| Batch Name | VG010522_8260B.batch.bin | Last Calib Update | 2/28/2022 2:48:47 PM |
| Ref Library | \\MASSHUNTER\Org\Library\NIST129K.I | | |



| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|--------------------|-------|----------|
| Internal Standards | | | | | | |
| M Fluorobenzene | 6.620 | 96.0 | 733634 | 250.0000 | ng | -0.003 |
| M Chlorobenzene-d5 | 9.774 | 82.0 | 287461 | 250.0000 | ng | 0.003 |
| M 1,4-Dichlorobenzene-d4 | 12.100 | 152.0 | 220029 | 250.0000 | ng | 0.000 |
| System Monitoring Compounds | | | | | | |
| S Dibromofluoromethane | 5.848 | 113.0 | 194240 | 281.0357 | ng | 0.003 |
| Spiked Amount: 250.000 | Range: 80.0 - 119.0% | | | Recovery = 112.41% | | |
| S 1,2-Dichloroethane-d4 | 6.233 | 67.0 | 85054 | 284.9092 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 81.0 - 118.0% | | | Recovery = 113.96% | | |
| S Toluene-d8 | 8.319 | 98.0 | 744246 | 268.6691 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 89.0 - 112.0% | | | Recovery = 107.47% | | |
| S p-Bromofluorobenzene | 10.954 | 95.0 | 217233 | 269.4934 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 85.0 - 114.0% | | | Recovery = 107.80% | | |
| Target Compounds | | | | | | |
| T Dichlorodifluoromethane | 0.000 | | 0 | N.D. | | |
| T Chloromethane | 1.417 | 50.0 | 1360 | 1.1653 | ng | m 96 |
| T Vinyl chloride | 0.000 | | 0 | N.D. | | |
| T Bromomethane | 0.000 | | 0 | N.D. | | |
| T Chloroethane | 0.000 | | 0 | N.D. | | |
| T Trichlorofluoromethane | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methylene chloride | 3.330 | 49.0 | 756 | 0.6936 | ng | m 83 |
| T trans-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methyl tert-butyl ether (MTBE) | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloroethane | 0.000 | | 0 | N.D. | | |
| T 2,2-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T cis-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methyl ethyl ketone | 0.000 | | 0 | N.D. | | |
| T Bromochloromethane | 0.000 | | 0 | N.D. | | |
| T Chloroform | 0.000 | | 0 | N.D. | | |


Quantitation Results Report (QT Reviewed)

| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|-----------------------------|-------|------|-------|-------|-------|----------|
| T 1,1,1-Trichloroethane | 0.000 | | 0 | N.D. | | |
| T Carbon tetrachloride | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloropropene | 0.000 | | 0 | N.D. | | |
| T Benzene | 0.000 | | 0 | N.D. | | |
| T 1,2-Dichloroethane | 0.000 | | 0 | N.D. | | |
| T Trichloroethene | 0.000 | | 0 | N.D. | | |
| T 1,2-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T Dibromomethane | 0.000 | | 0 | N.D. | | |
| T Bromodichloromethane | 0.000 | | 0 | N.D. | | |
| T cis-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | |
| T Toluene | 0.000 | | 0 | N.D. | | |
| T trans-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | |
| T 1,1,2-Trichloroethane | 0.000 | | 0 | N.D. | | |
| T Tetrachloroethene | 0.000 | | 0 | N.D. | | |
| T 1,3-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T Chlorodibromomethane | 0.000 | | 0 | N.D. | | |
| T 1,2-Dibromoethane | 0.000 | | 0 | N.D. | | |
| T Chlorobenzene | 0.000 | | 0 | N.D. | | |
| T 1,1,1,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | |
| T Ethylbenzene | 0.000 | | 0 | N.D. | | |
| T m+p-Xylenes | 0.000 | | 0 | N.D. | | |
| T o-Xylene | 0.000 | | 0 | N.D. | | |
| T Styrene | 0.000 | | 0 | N.D. | | |
| T Bromoform | 0.000 | | 0 | N.D. | | |
| T Bromobenzene | 0.000 | | 0 | N.D. | | |
| T 1,1,2,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | |
| T 1,2,3-Trichloropropane | 0.000 | | 0 | N.D. | | |
| T 2-Chlorotoluene | 0.000 | | 0 | N.D. | | |
| T 4-Chlorotoluene | 0.000 | | 0 | N.D. | | |
| T 1,3-Dichlorobenzene | 0.000 | | 0 | N.D. | | |
| T 1,4-Dichlorobenzene | 0.000 | | 0 | N.D. | | |
| T 1,2-Dichlorobenzene | 0.000 | | 0 | N.D. | | |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|-------------------------|-------|--------|------|-----------|
| Dichlorodifluoromethane | N.D. | 1.24 | 87.0 | 32.3 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------|--------|------|----------|----------|------|--------|-------|-------|
| Chloromethane | 1.1653 | 1.42 | 0.01 | 1360 (m) | 52.0 | 34.5 | 2.1 | 62.1 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------------|-------|--------|------|-----------|
| Vinyl chloride | N.D. | 1.50 | 64.0 | 29.9 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------|-------|--------|------|-----------|
| Bromomethane | N.D. | 1.80 | 94.0 | 104.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------|-------|--------|------|-----------|
| Chloroethane | N.D. | 1.89 | 66.0 | 30.1 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|------------------------|-------|--------|-------|-----------|
| Trichlorofluoromethane | N.D. | 2.14 | 103.0 | 64.2 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethene | N.D. | 2.70 | 61.0 | 180.3 | 63.0 | 56.7 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|--------|------|----------|---------|------|--------|-------|-------|
| Methylene chloride | 0.6936 | 3.33 | -0.01 | 756 (m) | 84.0 | 59.5 | 36.9 | 96.9 |
| | | | | | 86.0 | 25.8 | 14.3 | 74.3 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,2-Dichloroethene | N.D. | 3.72 | 61.0 | 153.9 | 98.0 | 65.7 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------------------|-------|--------|------|-----------|
| Methyl tert-butyl ether (MTBE) | N.D. | 3.75 | 57.0 | 24.6 |











| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethane | N.D. | 4.38 | 65.0 | 32.1 | 83.0 | 13.7 |







| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|------|-----------|
| 2,2-Dichloropropane | N.D. | 5.20 | 41.0 | 66.5 | 97.0 | 23.2 |



Quantitation Results Report (QT Reviewed)

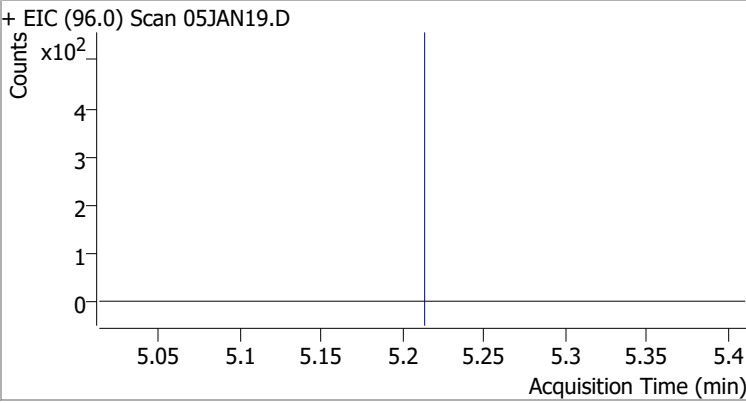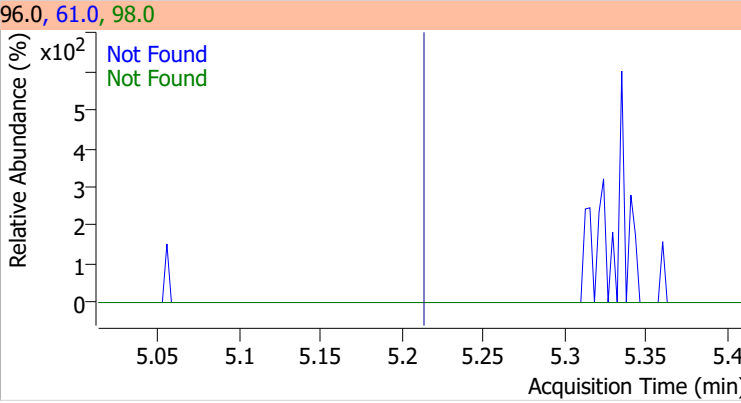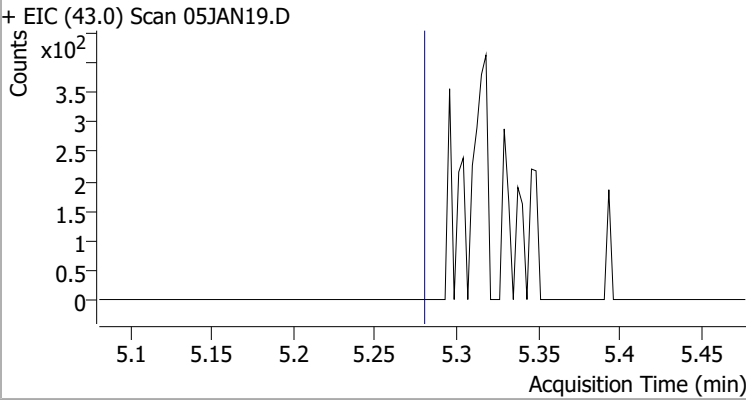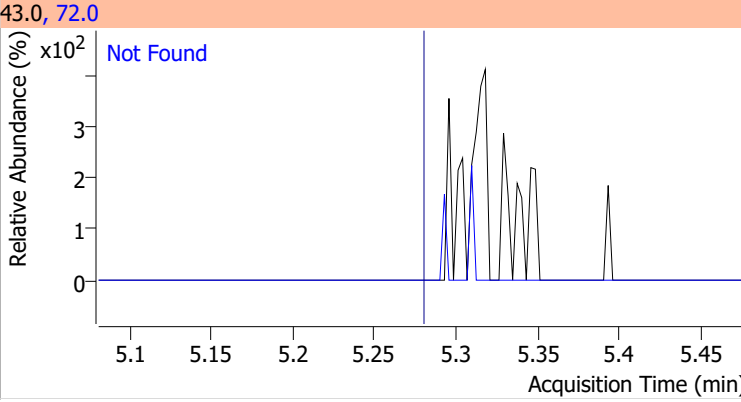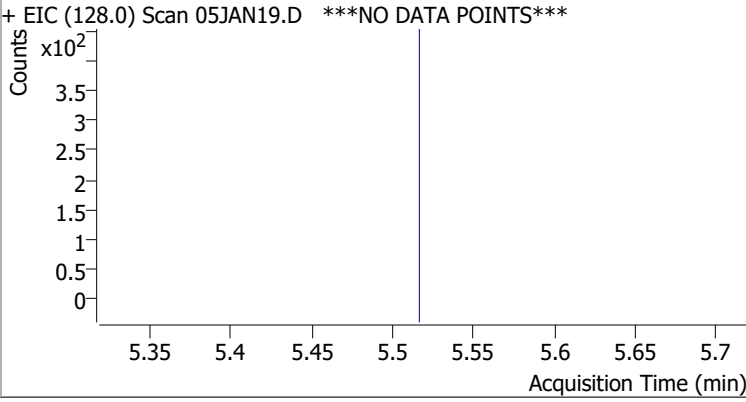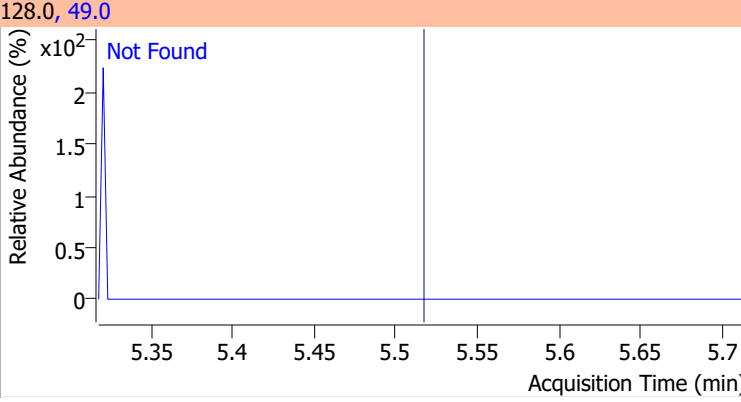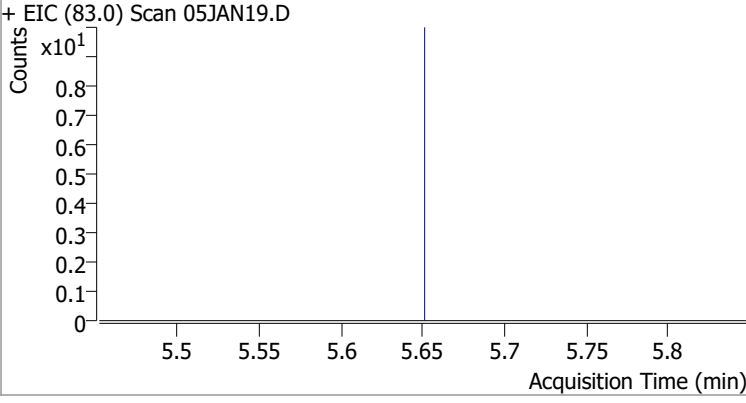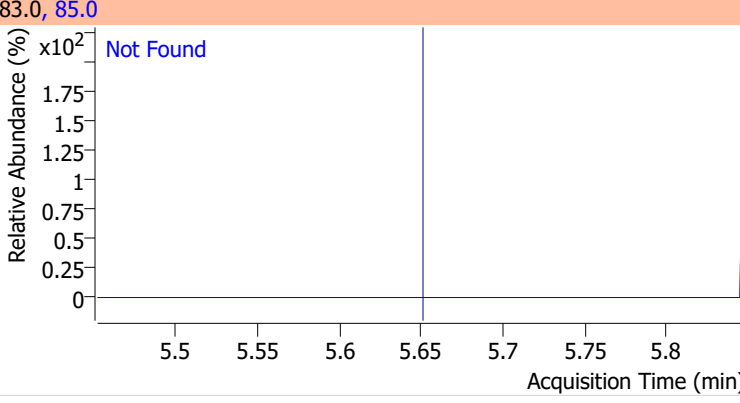
| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--|-------|--------|--|-----------|------|-----------|
| cis-1,2-Dichloroethene | N.D. | 5.22 | 61.0 | 167.2 | 98.0 | 67.3 |
| + EIC (96.0) Scan 05JAN19.D | | | 96.0, 61.0, 98.0 | | | |
|  | | |  | | | |
| Methyl ethyl ketone | N.D. | 5.28 | 72.0 | 21.3 | | |
| + EIC (43.0) Scan 05JAN19.D | | | 43.0, 72.0 | | | |
|  | | |  | | | |
| Bromochloromethane | N.D. | 5.52 | 49.0 | 182.9 | | |
| + EIC (128.0) Scan 05JAN19.D ***NO DATA POINTS*** | | | 128.0, 49.0 | | | |
|  | | |  | | | |
| Chloroform | N.D. | 5.65 | 85.0 | 66.0 | | |
| + EIC (83.0) Scan 05JAN19.D | | | 83.0, 85.0 | | | |
|  | | |  | | | |

Quantitation Results Report (QT Reviewed)

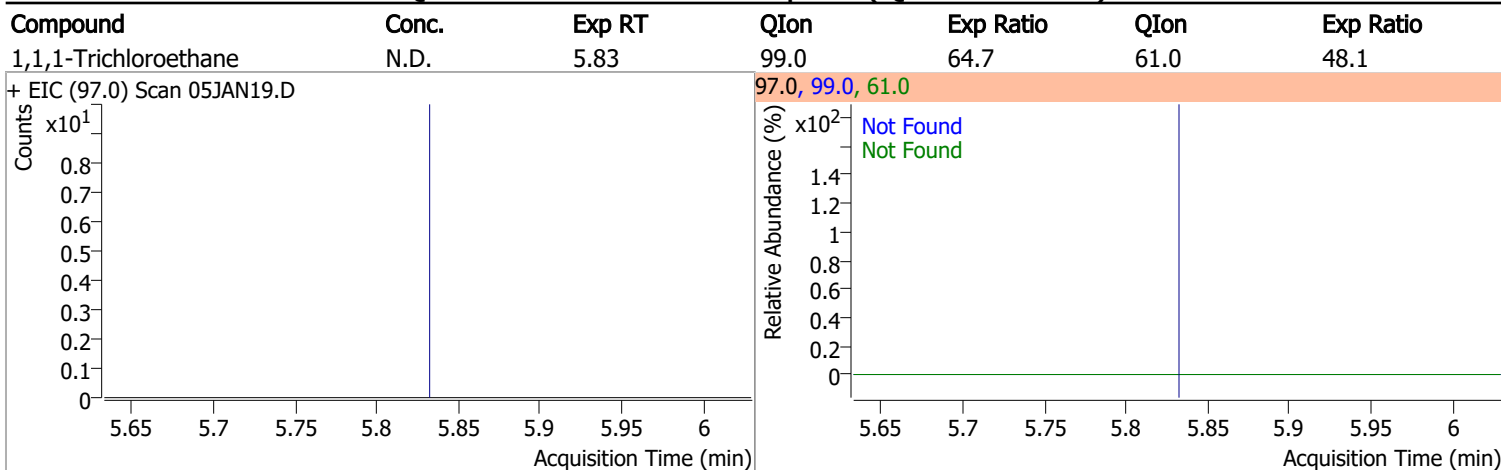


Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 284.9092 | 6.23 | 0.00 | 85054 | 65.0 | 202.4 | 166.5 | 226.5 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------|-------|--------|------|-----------|
| Benzene | N.D. | 6.28 | 77.0 | 23.5 |







| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,2-Dichloroethane | N.D. | 6.32 | 64.0 | 29.9 | 98.0 | 7.6 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------|-------|--------|-------|-----------|------|-----------|
| Trichloroethene | N.D. | 7.03 | 130.0 | 101.5 | 97.0 | 64.1 |




Quantitation Results Report (QT Reviewed)

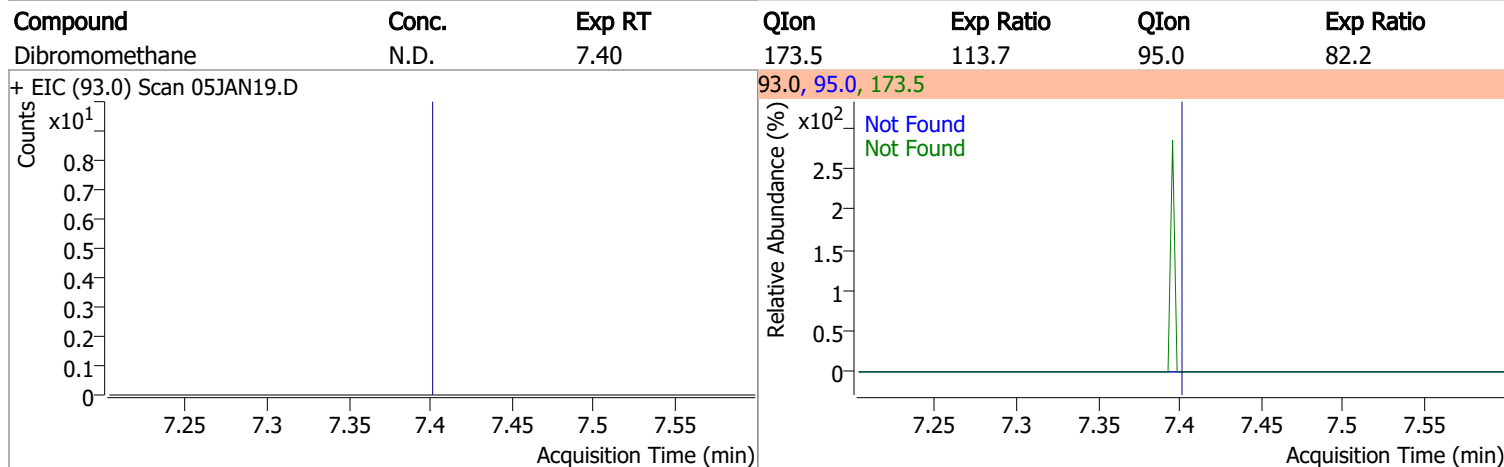


Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 268.6691 | 8.32 | 0.00 | 744246 | 100.0 | 63.5 | 34.4 | 94.4 |
| | | | | | 99.0 | 9.4 | 0.0 | 39.6 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------|-------|--------|------|-----------|
| Toluene | N.D. | 8.39 | 91.0 | 175.8 |











| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,3-Dichloropropene | N.D. | 8.64 | 39.0 | 53.4 | 77.0 | 32.4 |











| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------------|-------|--------|------|-----------|------|-----------|
| 1,1,2-Trichloroethane | N.D. | 8.82 | 97.0 | 114.6 | 85.0 | 67.6 |






Quantitation Results Report (QT Reviewed)
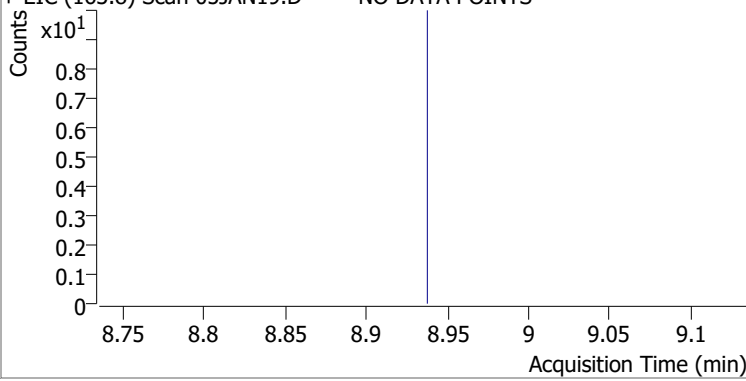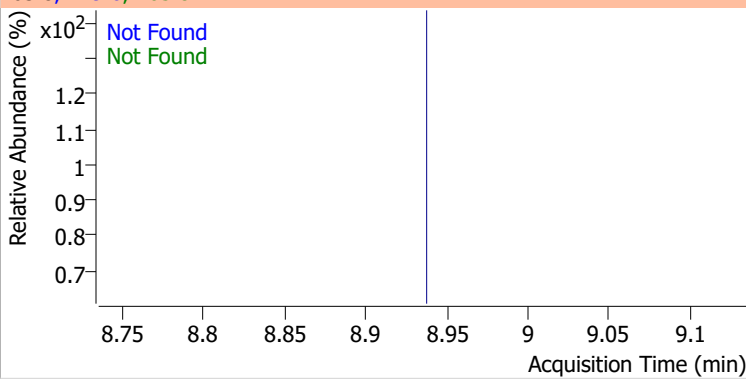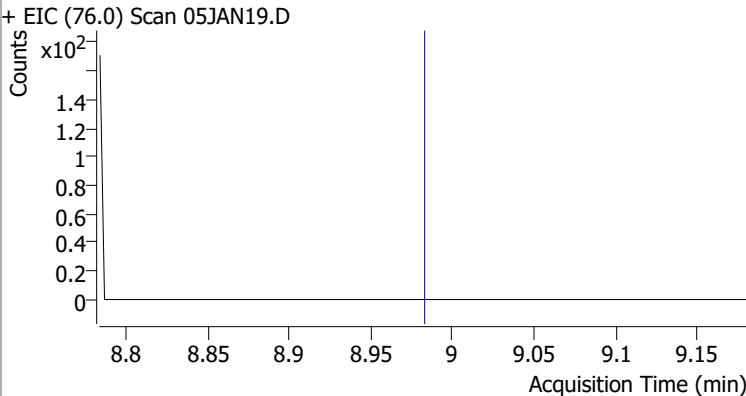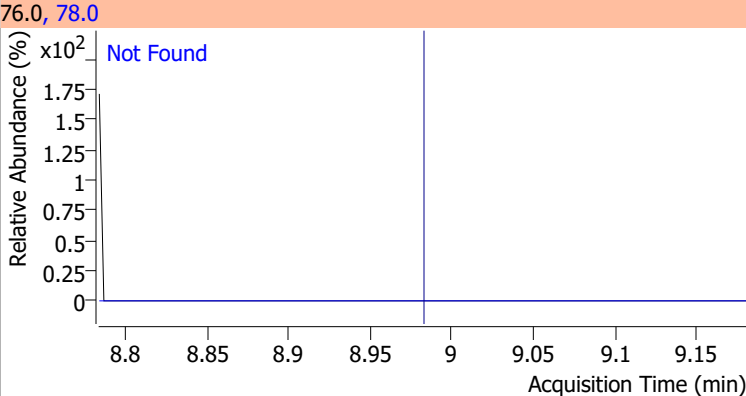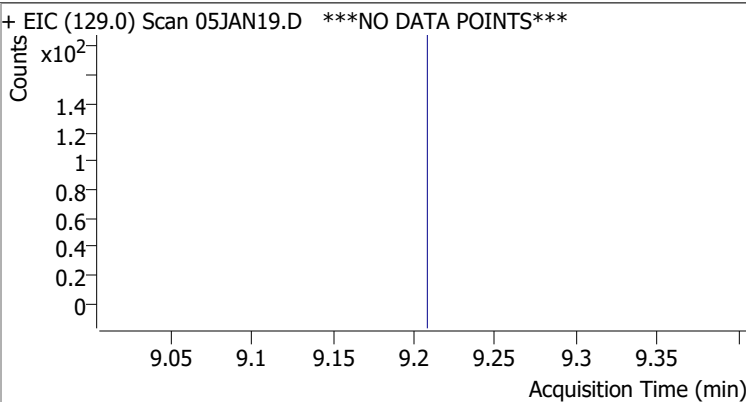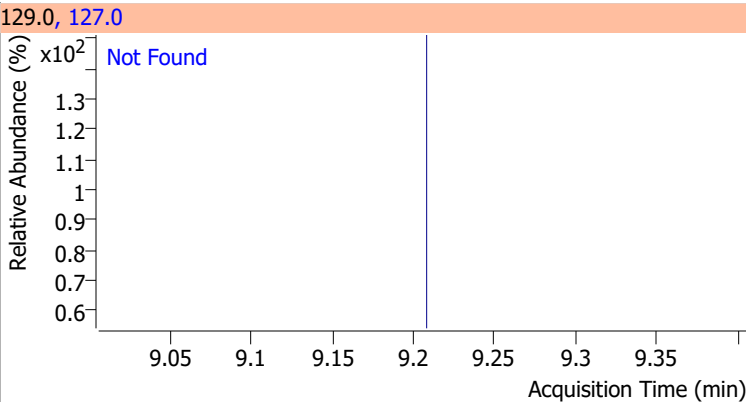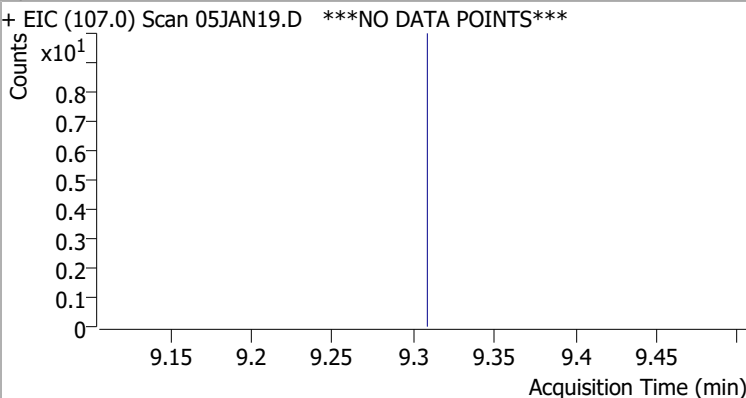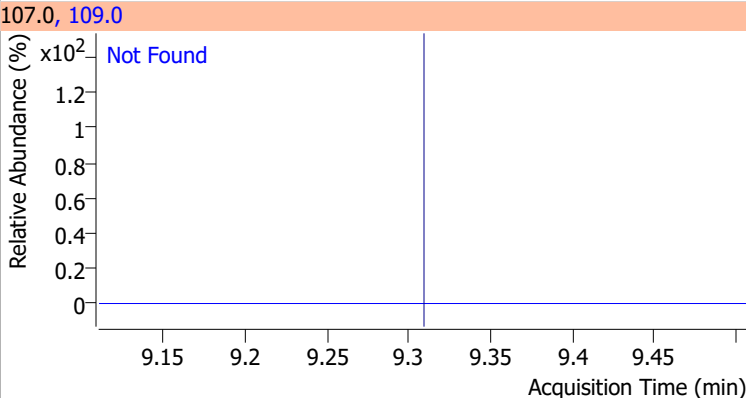
| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--|-------|--------|--|-----------|-------|-----------|
| Tetrachloroethene | N.D. | 8.94 | 165.8 | 128.6 | 129.0 | 91.5 |
| + EIC (163.8) Scan 05JAN19.D ***NO DATA POINTS*** | | | 163.8, 129.0, 165.8 | | | |
|  | | |  | | | |
| 1,3-Dichloropropane | N.D. | 8.98 | 78.0 | 32.9 | | |
| + EIC (76.0) Scan 05JAN19.D | | | 76.0, 78.0 | | | |
|  | | |  | | | |
| Chlorodibromomethane | N.D. | 9.21 | 127.0 | 78.0 | | |
| + EIC (129.0) Scan 05JAN19.D ***NO DATA POINTS*** | | | 129.0, 127.0 | | | |
|  | | |  | | | |
| 1,2-Dibromoethane | N.D. | 9.31 | 109.0 | 94.5 | | |
| + EIC (107.0) Scan 05JAN19.D ***NO DATA POINTS*** | | | 107.0, 109.0 | | | |
|  | | |  | | | |


Quantitation Results Report (QT Reviewed)
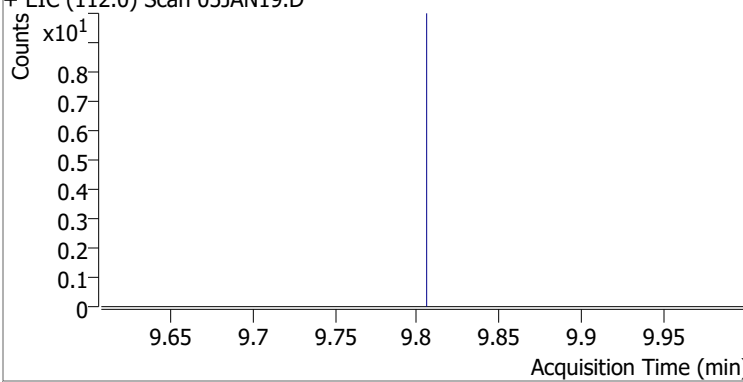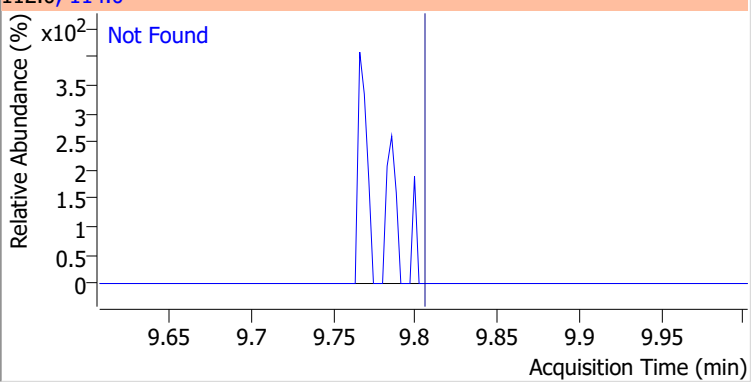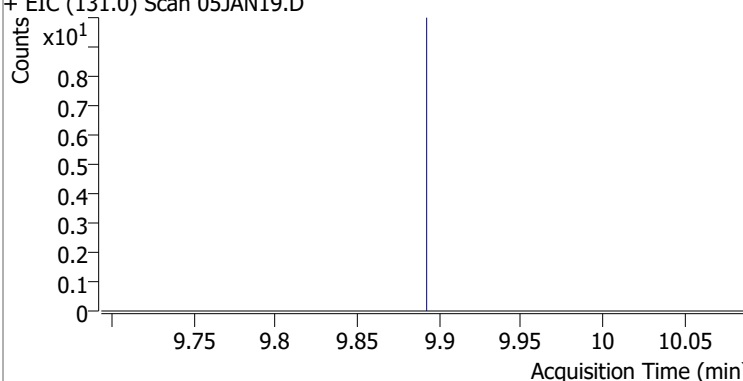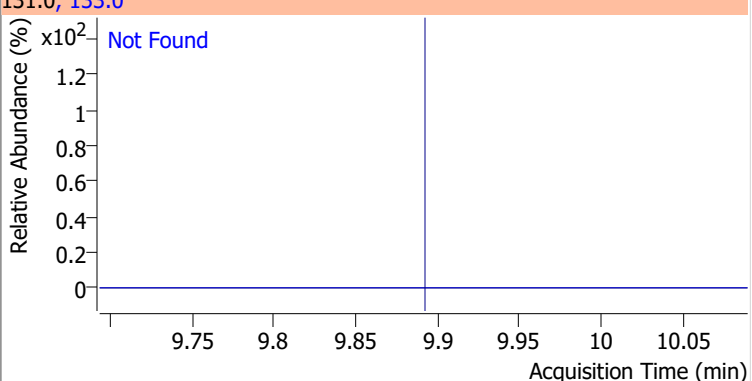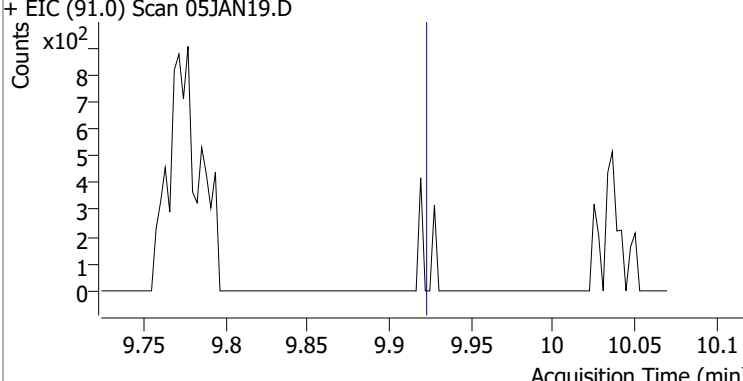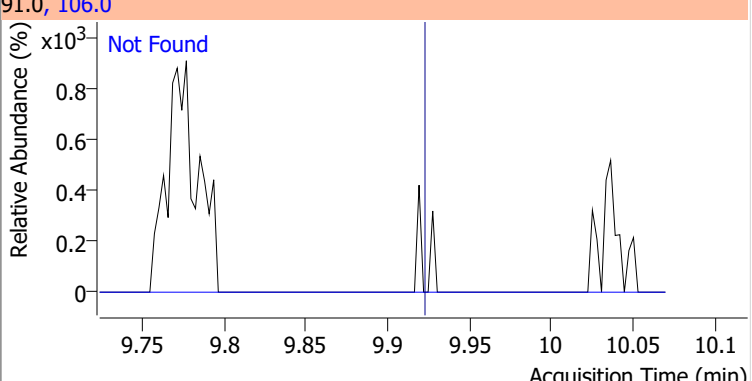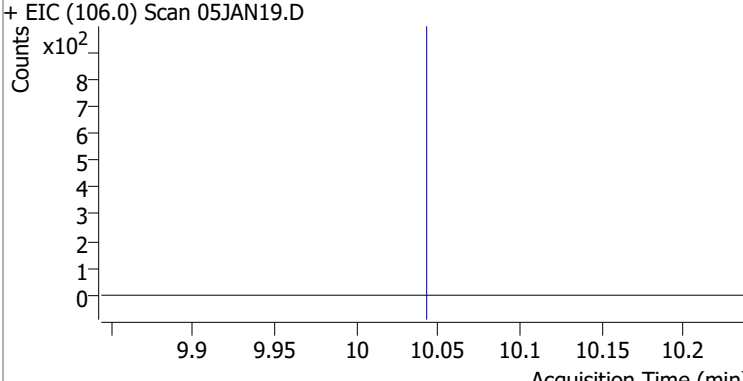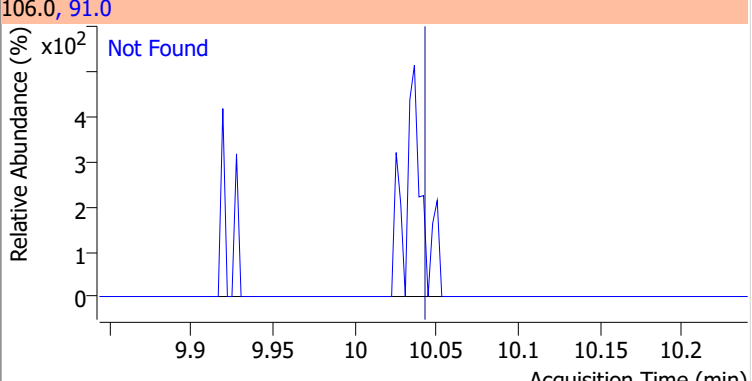
| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--|-------|--------|--|-----------|
| Chlorobenzene | N.D. | 9.80 | 114.0 | 32.1 |
| + EIC (112.0) Scan 05JAN19.D | | | 112.0, 114.0 | |
|  | | |  | |
| 1,1,1,2-Tetrachloroethane | N.D. | 9.89 | 133.0 | 98.6 |
| + EIC (131.0) Scan 05JAN19.D | | | 131.0, 133.0 | |
|  | | |  | |
| Ethylbenzene | N.D. | 9.92 | 106.0 | 31.1 |
| + EIC (91.0) Scan 05JAN19.D | | | 91.0, 106.0 | |
|  | | |  | |
| m+p-Xylenes | N.D. | 10.04 | 91.0 | 201.4 |
| + EIC (106.0) Scan 05JAN19.D | | | 106.0, 91.0 | |
|  | | |  | |









Quantitation Results Report (QT Reviewed)

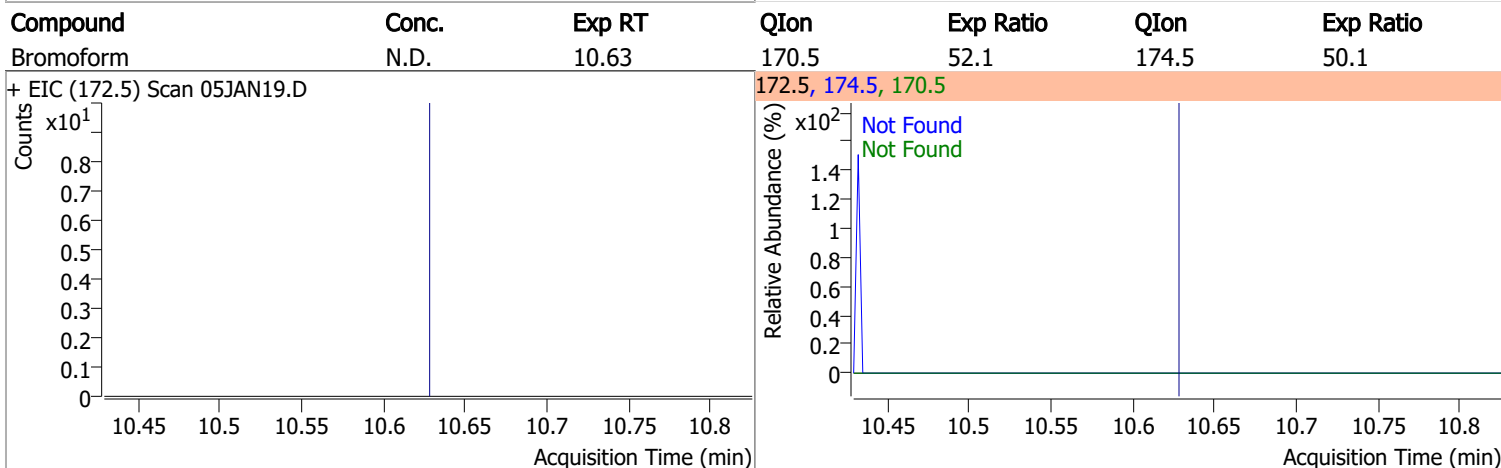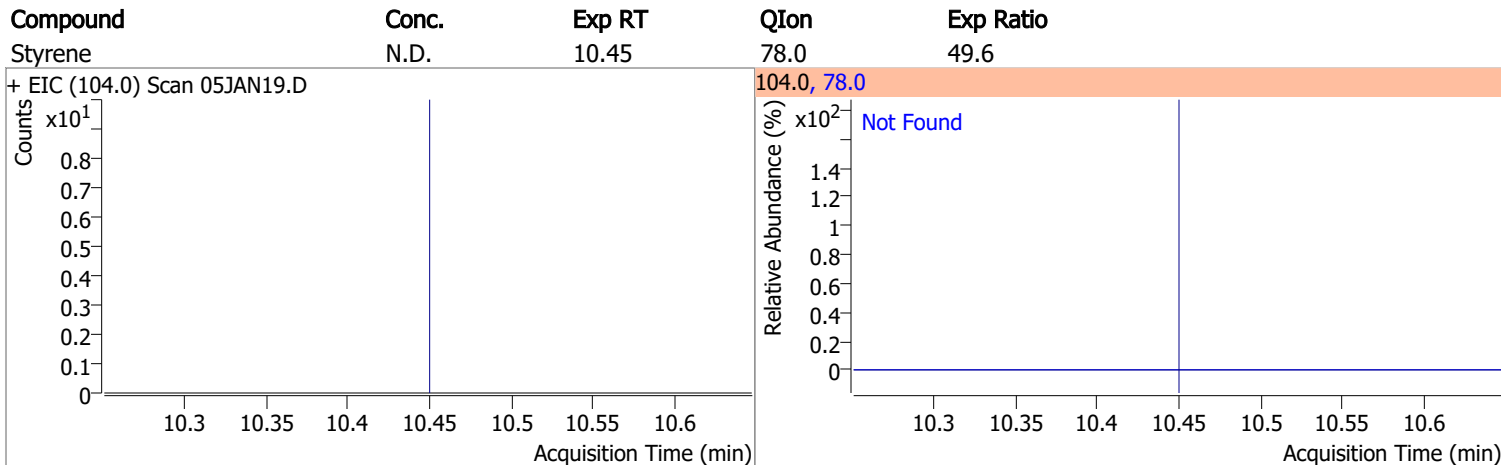









| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 269.4934 | 10.95 | 0.00 | 217233 | 174.0 | 93.5 | 61.7 | 121.7 |
| | | | | | 176.0 | 91.5 | 60.6 | 120.6 |



Quantitation Results Report (QT Reviewed)

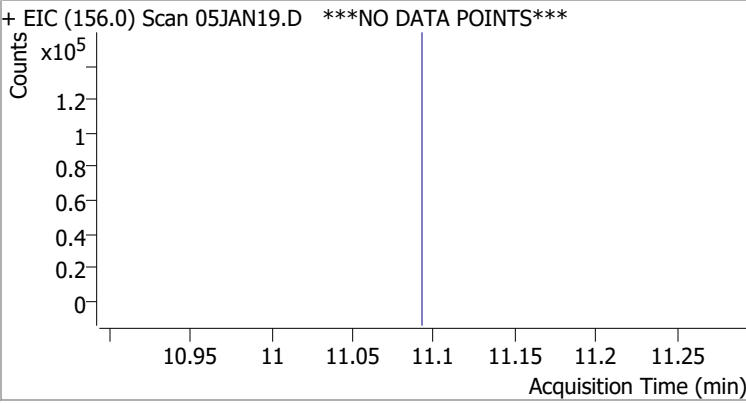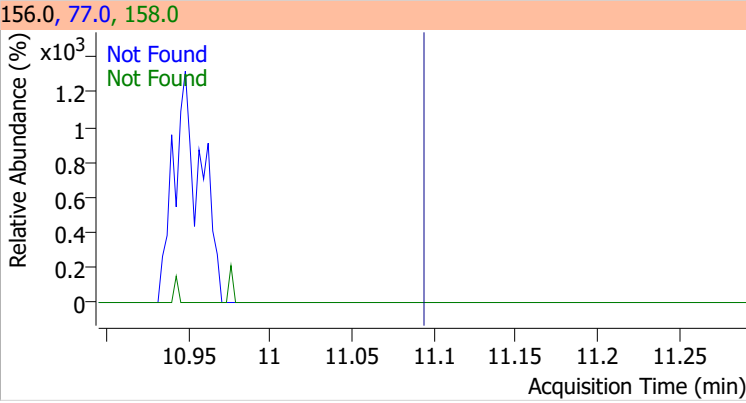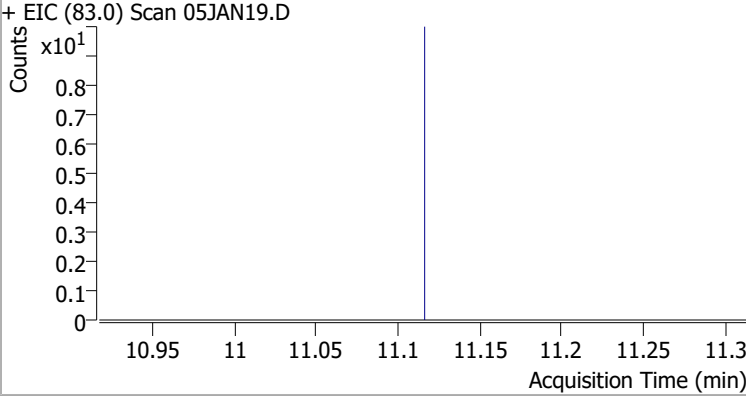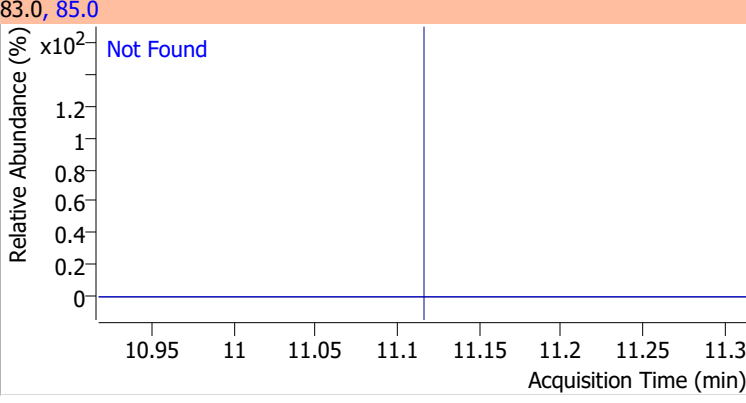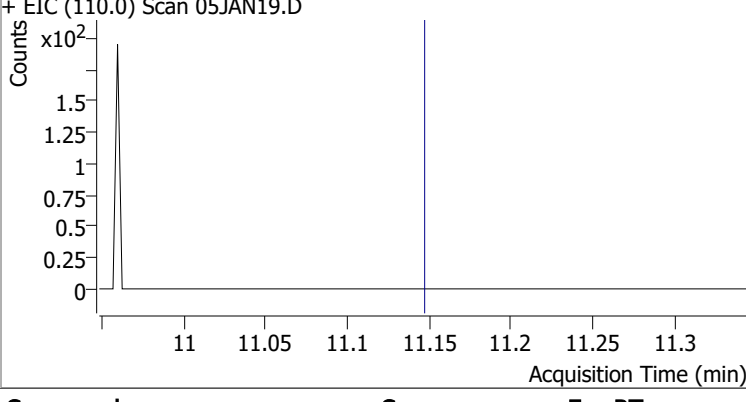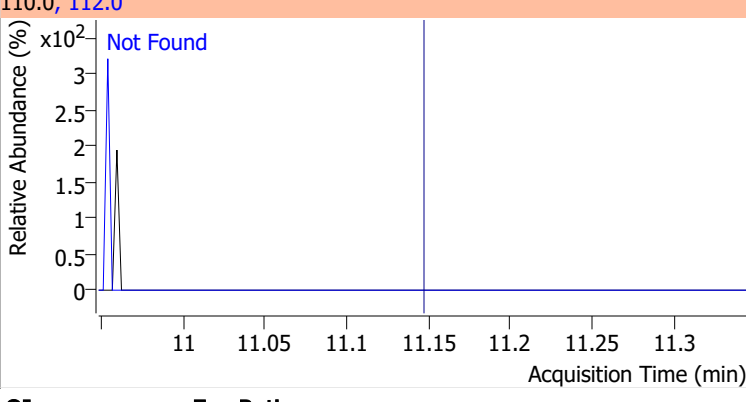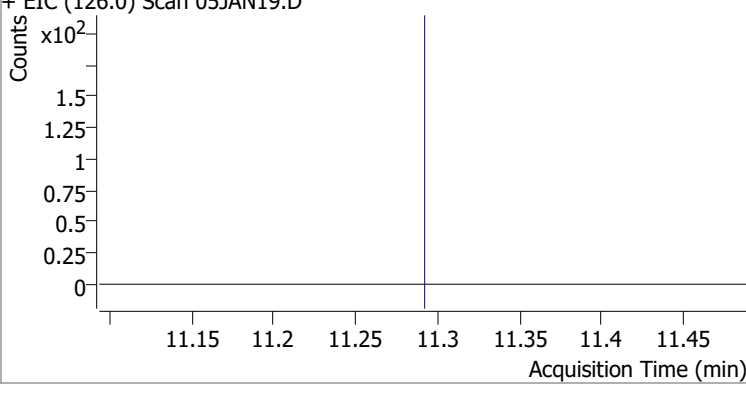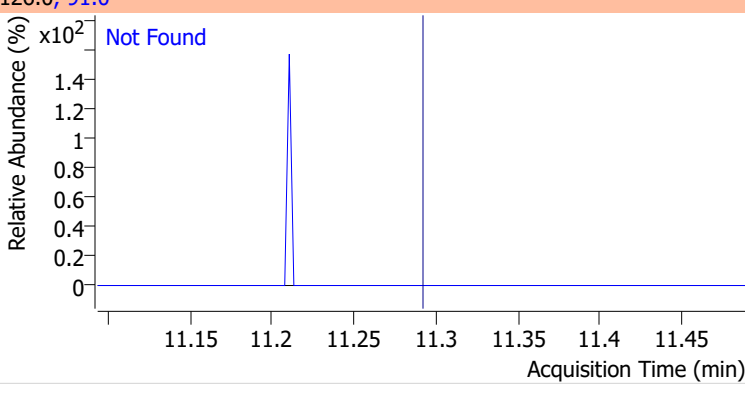
| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--|-------|--------|--|-----------|-------|-----------|
| Bromobenzene | N.D. | 11.09 | 77.0 | 145.7 | 158.0 | 96.5 |
| + EIC (156.0) Scan 05JAN19.D ***NO DATA POINTS*** | | | 156.0, 77.0, 158.0 | | | |
|  | | |  | | | |
| 1,1,2,2-Tetrachloroethane | N.D. | 11.12 | 85.0 | 66.2 | | |
| + EIC (83.0) Scan 05JAN19.D | | | 83.0, 85.0 | | | |
|  | | |  | | | |
| 1,2,3-Trichloropropane | N.D. | 11.15 | 112.0 | 63.5 | | |
| + EIC (110.0) Scan 05JAN19.D | | | 110.0, 112.0 | | | |
|  | | |  | | | |
| 2-Chlorotoluene | N.D. | 11.29 | 91.0 | 282.3 | | |
| + EIC (126.0) Scan 05JAN19.D | | | 126.0, 91.0 | | | |
|  | | |  | | | |

Quantitation Results Report (QT Reviewed)
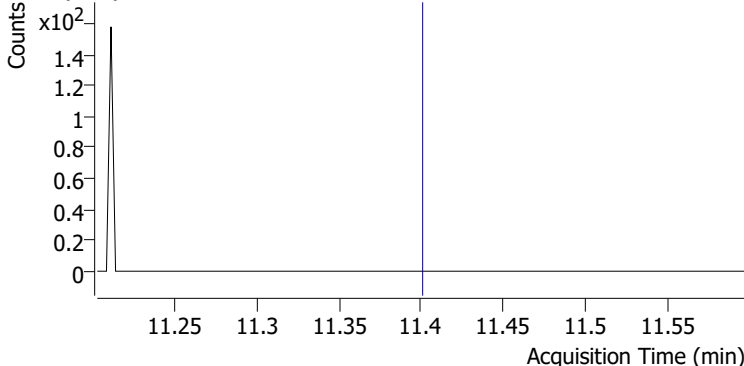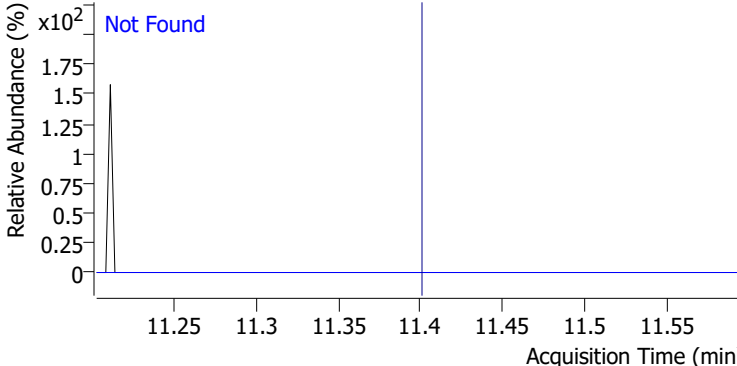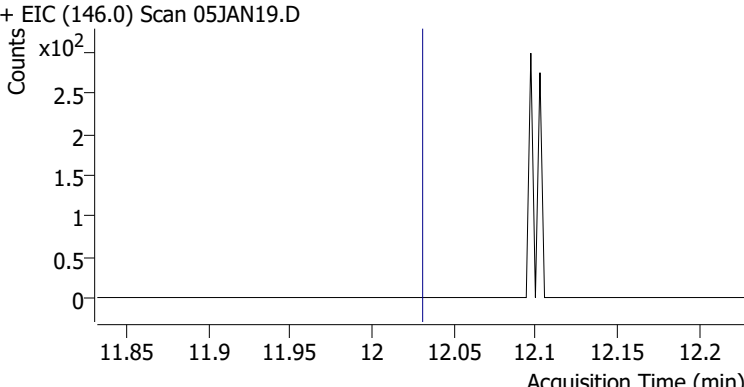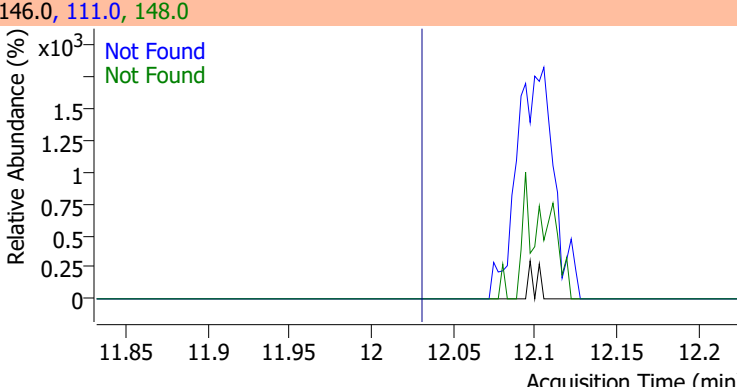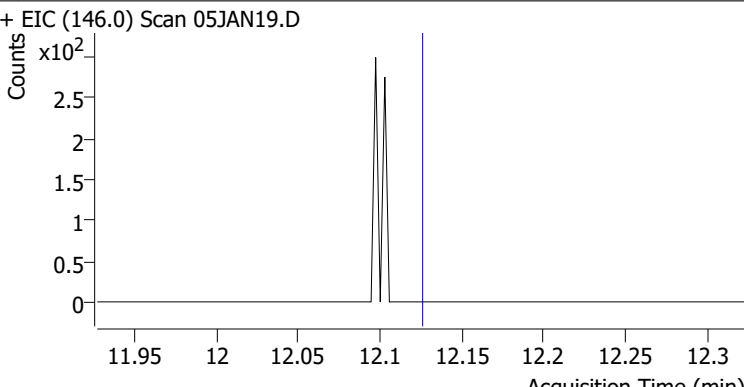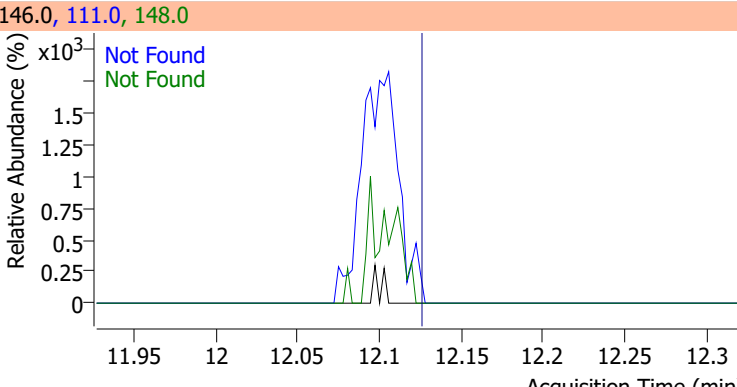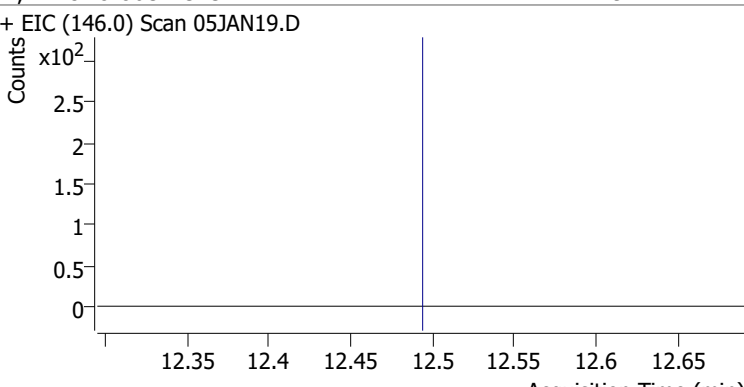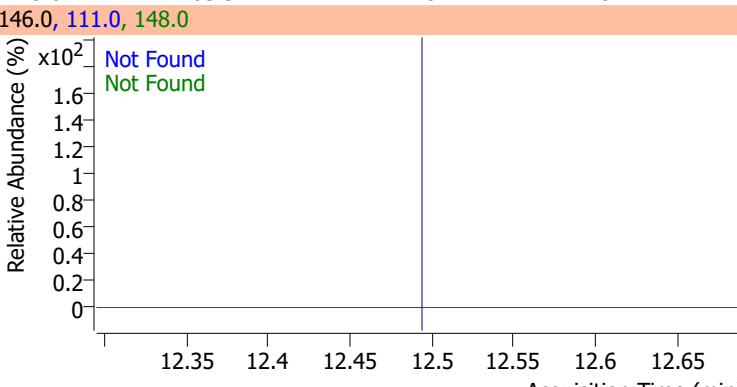
| Compound | Conc. | Exp RT | QIon | Exp Ratio | | |
|--|-------|--------|--|-----------|------|-----------|
| 4-Chlorotoluene | N.D. | 11.40 | 126.0 | 31.7 | | |
| + EIC (91.0) Scan 05JAN19.D | | | 91.0, 126.0 | | | |
|  | | |  | | | |
| 1,3-Dichlorobenzene | N.D. | 12.03 | 148.0 | 63.6 | QIon | Exp Ratio |
| + EIC (146.0) Scan 05JAN19.D | | | 146.0, 111.0, 148.0 | | | |
|  | | |  | | | |
| 1,4-Dichlorobenzene | N.D. | 12.13 | 148.0 | 63.1 | QIon | Exp Ratio |
| + EIC (146.0) Scan 05JAN19.D | | | 146.0, 111.0, 148.0 | | | |
|  | | |  | | | |
| 1,2-Dichlorobenzene | N.D. | 12.49 | 148.0 | 63.9 | QIon | Exp Ratio |
| + EIC (146.0) Scan 05JAN19.D | | | 146.0, 111.0, 148.0 | | | |
|  | | |  | | | |

Quantitation Results Report (QT Reviewed)

| | | | |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File | 05JAN20.D | Operator | MSC |
| Acq. Method | 5975CACQF.M | Acq. Date-Time | 1/5/2022 6:44:10 PM |
| Sample Name | B22010141-001F | Instrument | VOA5975C |
| Vial | 20 | Multiplier | 1.00 |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m | Comment | |
| Tune File | BFB_Atune3.u | Tune Date | 10/11/2021 4:02:00 PM |
| Batch Name | VG010522_8260B.batch.bin | Last Calib Update | 2/28/2022 2:48:47 PM |
| Ref Library | \\MASSHUNTER\Org\Library\NIST129K.I | | |



| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|----------|----|------|-------|-------|-------|----------|
|----------|----|------|-------|-------|-------|----------|

Internal Standards

| | | | | | | |
|--------------------------|--------|-------|--------|----------|----|--------|
| M Fluorobenzene | 6.620 | 96.0 | 736081 | 250.0000 | ng | -0.003 |
| M Chlorobenzene-d5 | 9.774 | 82.0 | 285810 | 250.0000 | ng | 0.003 |
| M 1,4-Dichlorobenzene-d4 | 12.100 | 152.0 | 218523 | 250.0000 | ng | 0.000 |

System Monitoring Compounds

| | | | | | | |
|-------------------------|----------------------|-------|--------|--------------------|----|-------|
| S Dibromofluoromethane | 5.848 | 113.0 | 192434 | 277.4972 | ng | 0.003 |
| Spiked Amount: 250.000 | Range: 80.0 - 119.0% | | | Recovery = 111.00% | | |
| S 1,2-Dichloroethane-d4 | 6.233 | 67.0 | 86001 | 287.1237 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 81.0 - 118.0% | | | Recovery = 114.85% | | |
| S Toluene-d8 | 8.321 | 98.0 | 735346 | 266.9897 | ng | 0.003 |
| Spiked Amount: 250.000 | Range: 89.0 - 112.0% | | | Recovery = 106.80% | | |
| S p-Bromofluorobenzene | 10.954 | 95.0 | 212642 | 265.6160 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 85.0 - 114.0% | | | Recovery = 106.25% | | |

Target Compounds









| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) | QValue |
|----------------------------------|-------|------|-------|-------|-------|----------|--------|
| T Dichlorodifluoromethane | 0.000 | | 0 | N.D. | | | |
| T Chloromethane | 0.000 | | 0 | N.D. | | | |
| T Vinyl chloride | 0.000 | | 0 | N.D. | | | |
| T Bromomethane | 0.000 | | 0 | N.D. | | | |
| T Chloroethane | 0.000 | | 0 | N.D. | | | |
| T Trichlorofluoromethane | 0.000 | | 0 | N.D. | | | |
| T 1,1-Dichloroethene | 0.000 | | 0 | N.D. | | | |
| T Methylene chloride | 0.000 | | 0 | N.D. | | | |
| T trans-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | | |
| T Methyl tert-butyl ether (MTBE) | 0.000 | | 0 | N.D. | | | |
| T 1,1-Dichloroethane | 0.000 | | 0 | N.D. | | | |
| T 2,2-Dichloropropane | 0.000 | | 0 | N.D. | | | |
| T cis-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | | |
| T Methyl ethyl ketone | 0.000 | | 0 | N.D. | | | |
| T Bromochloromethane | 0.000 | | 0 | N.D. | | | |
| T Chloroform | 0.000 | | 0 | N.D. | | | |

Quantitation Results Report (QT Reviewed)









| Compound | RT | QIon | Resp. | Conc. | Units | | Dev(Min) |
|-----------------------------|--------|-------|-------|--------|-------|----|----------|
| T 1,1,1-Trichloroethane | 0.000 | | 0 | N.D. | | | |
| T Carbon tetrachloride | 0.000 | | 0 | N.D. | | | |
| T 1,1-Dichloropropene | 0.000 | | 0 | N.D. | | | |
| T Benzene | 6.277 | 78.0 | 427 | 0.1455 | ng | m | 85 |
| T 1,2-Dichloroethane | 0.000 | | 0 | N.D. | | | |
| T Trichloroethene | 0.000 | | 0 | N.D. | | | |
| T 1,2-Dichloropropane | 0.000 | | 0 | N.D. | | | |
| T Dibromomethane | 0.000 | | 0 | N.D. | | | |
| T Bromodichloromethane | 0.000 | | 0 | N.D. | | | |
| T cis-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | | |
| T Toluene | 0.000 | | 0 | N.D. | | | |
| T trans-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | | |
| T 1,1,2-Trichloroethane | 0.000 | | 0 | N.D. | | | |
| T Tetrachloroethene | 0.000 | | 0 | N.D. | | | |
| T 1,3-Dichloropropane | 0.000 | | 0 | N.D. | | | |
| T Chlorodibromomethane | 0.000 | | 0 | N.D. | | | |
| T 1,2-Dibromoethane | 0.000 | | 0 | N.D. | | | |
| T Chlorobenzene | 0.000 | | 0 | N.D. | | | |
| T 1,1,1,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | | |
| T Ethylbenzene | 0.000 | | 0 | N.D. | | | |
| T m+p-Xylenes | 10.048 | 106.0 | 0 | | ng | md | 1 |
| T o-Xylene | 0.000 | | 0 | N.D. | | | |
| T Styrene | 0.000 | | 0 | N.D. | | | |
| T Bromoform | 0.000 | | 0 | N.D. | | | |
| T Bromobenzene | 0.000 | | 0 | N.D. | | | |
| T 1,1,2,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | | |
| T 1,2,3-Trichloropropane | 0.000 | | 0 | N.D. | | | |
| T 2-Chlorotoluene | 0.000 | | 0 | N.D. | | | |
| T 4-Chlorotoluene | 0.000 | | 0 | N.D. | | | |
| T 1,3-Dichlorobenzene | 0.000 | | 0 | N.D. | | | |
| T 1,4-Dichlorobenzene | 0.000 | | 0 | N.D. | | | |
| T 1,2-Dichlorobenzene | 0.000 | | 0 | N.D. | | | |

(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)

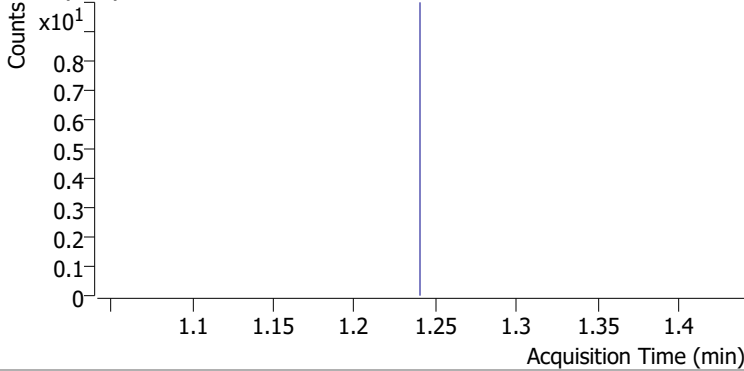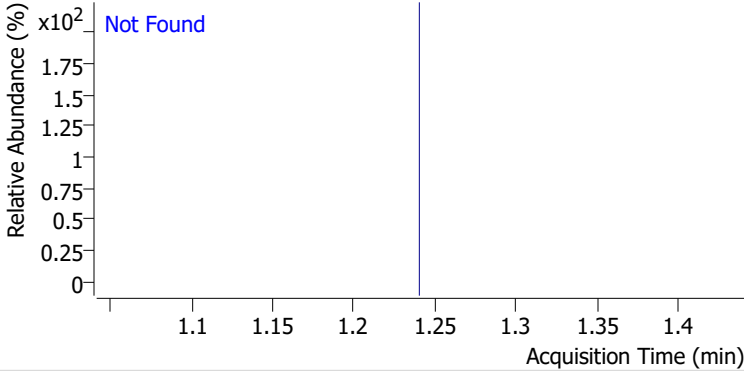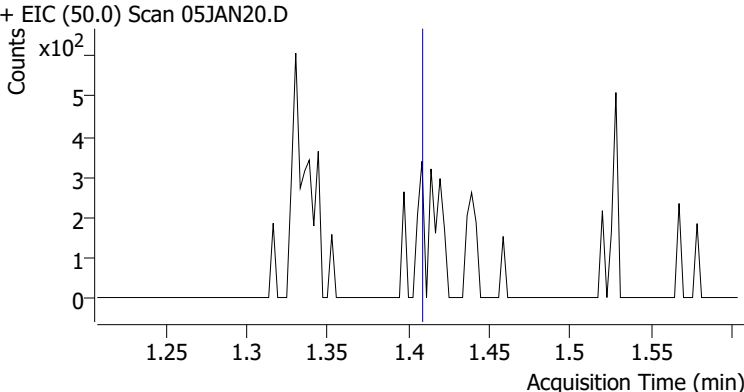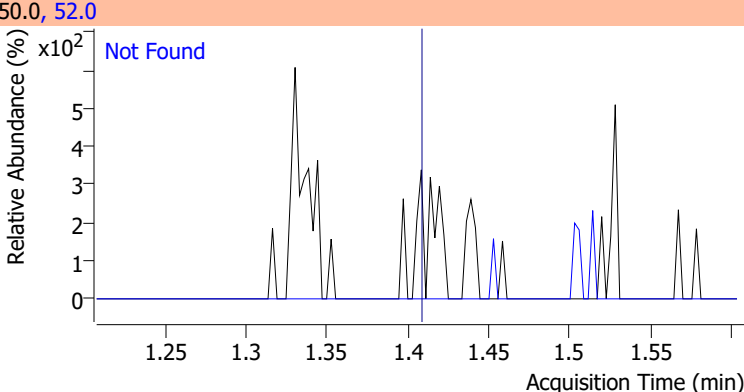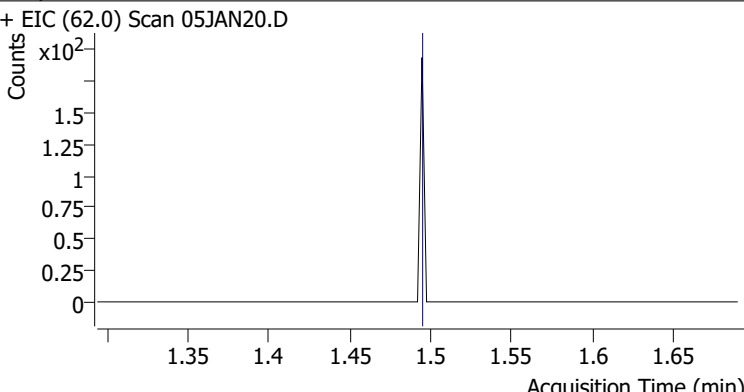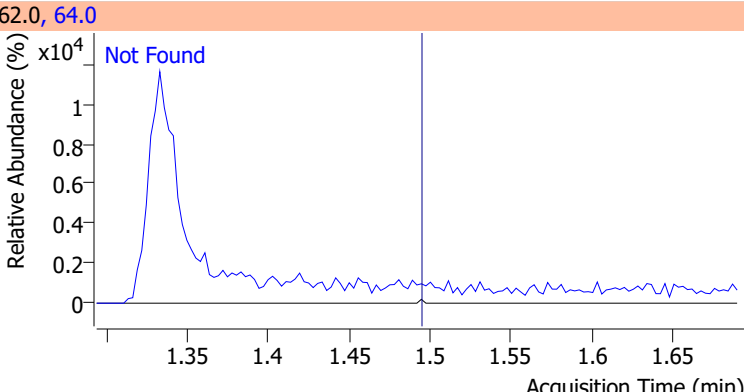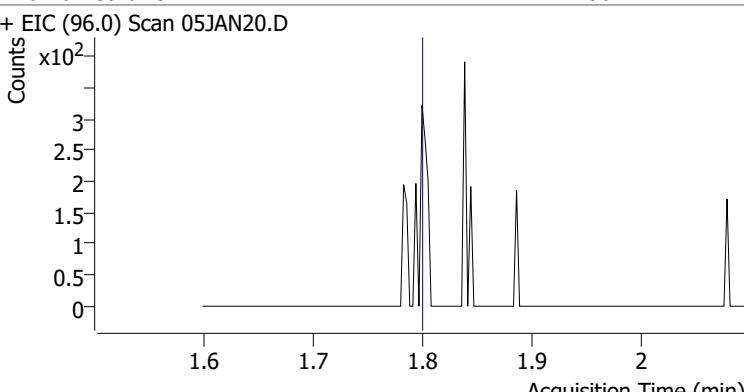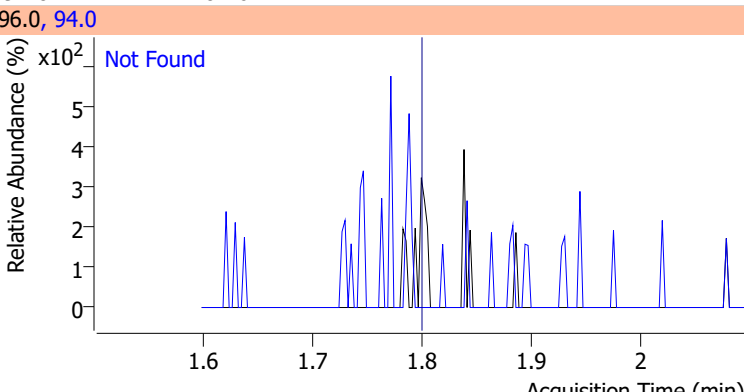
| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--|-------|--------|--|-----------|
| Dichlorodifluoromethane | N.D. | 1.24 | 87.0 | 32.3 |
| + EIC (85.0) Scan 05JAN20.D ***NO DATA POINTS*** | | | 85.0, 87.0 | |
|  | | |  | |
| Chloromethane | N.D. | 1.41 | 52.0 | 32.1 |
| + EIC (50.0) Scan 05JAN20.D | | | 50.0, 52.0 | |
|  | | |  | |
| Vinyl chloride | N.D. | 1.50 | 64.0 | 29.9 |
| + EIC (62.0) Scan 05JAN20.D | | | 62.0, 64.0 | |
|  | | |  | |
| Bromomethane | N.D. | 1.80 | 94.0 | 104.6 |
| + EIC (96.0) Scan 05JAN20.D | | | 96.0, 94.0 | |
|  | | |  | |

Quantitation Results Report (QT Reviewed)

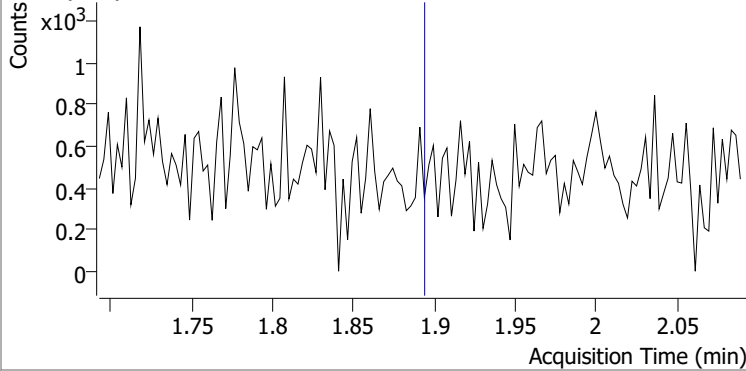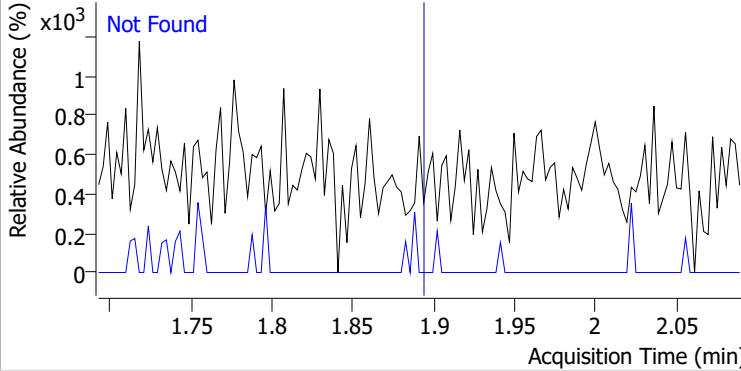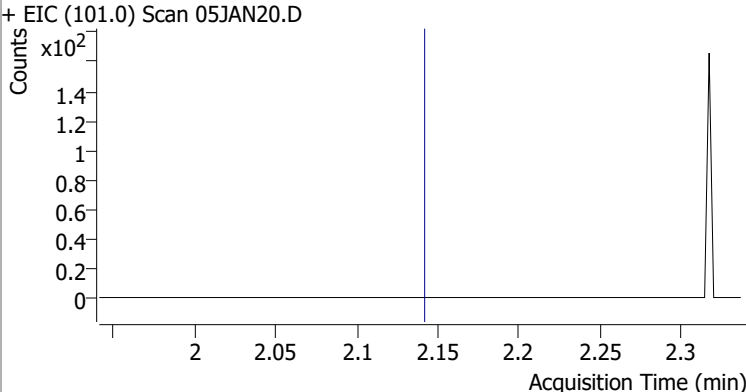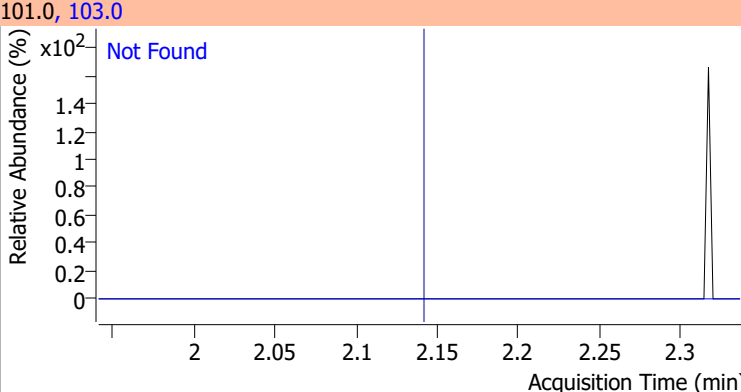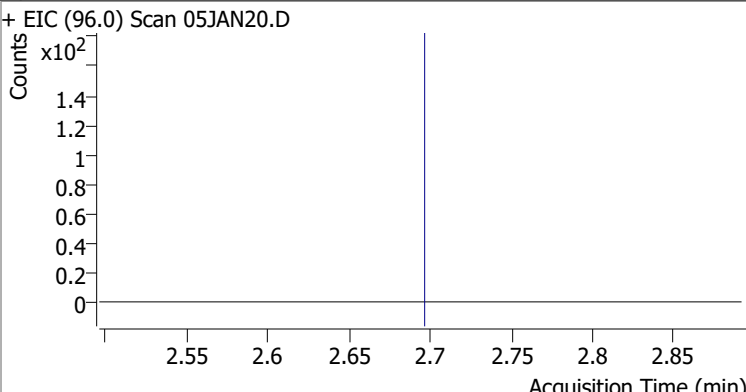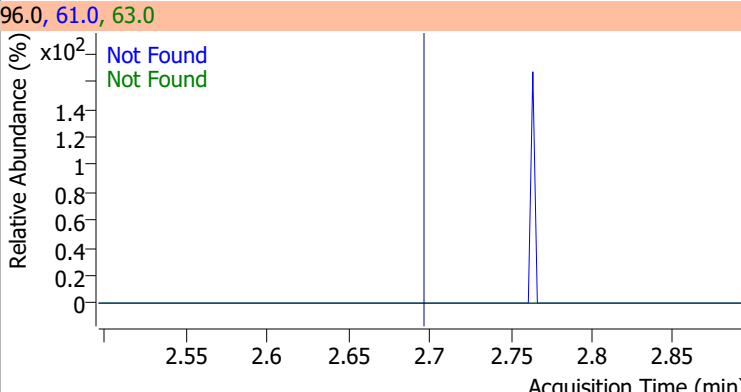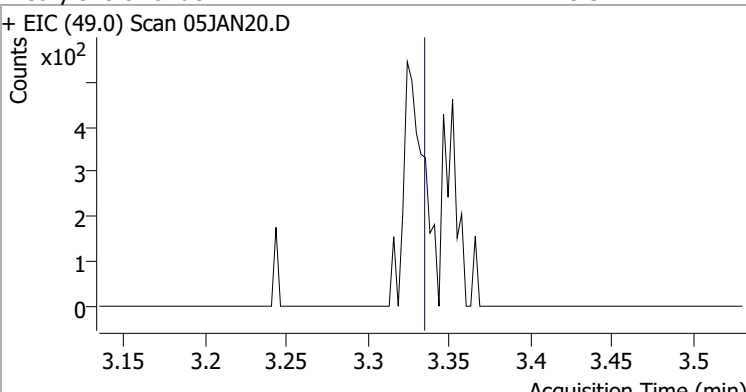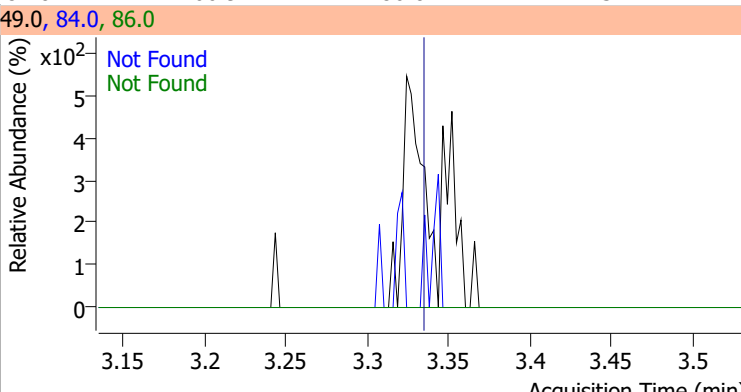
| Compound | Conc. | Exp RT | QIon | Exp Ratio | | |
|--|--|--------|------------------|-----------|------|-----------|
| Chloroethane | N.D. | 1.89 | 66.0 | 30.1 | | |
| + EIC (64.0) Scan 05JAN20.D | | | 64.0, 66.0 | | | |
|  |  | | | | | |
| Trichlorofluoromethane | N.D. | 2.14 | 103.0 | 64.2 | | |
| + EIC (101.0) Scan 05JAN20.D | | | 101.0, 103.0 | | | |
|  |  | | | | | |
| 1,1-Dichloroethene | N.D. | 2.70 | 61.0 | 180.3 | QIon | Exp Ratio |
| | | | | | 63.0 | 56.7 |
| + EIC (96.0) Scan 05JAN20.D | | | 96.0, 61.0, 63.0 | | | |
|  |  | | | | | |
| Methylene chloride | N.D. | 3.34 | 84.0 | 66.9 | QIon | Exp Ratio |
| | | | | | 86.0 | 44.3 |
| + EIC (49.0) Scan 05JAN20.D | | | 49.0, 84.0, 86.0 | | | |
|  |  | | | | | |

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,2-Dichloroethene | N.D. | 3.72 | 61.0 | 153.9 | 98.0 | 65.7 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------------------|-------|--------|------|-----------|
| Methyl tert-butyl ether (MTBE) | N.D. | 3.75 | 57.0 | 24.6 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethane | N.D. | 4.38 | 65.0 | 32.1 | 83.0 | 13.7 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|------|-----------|
| 2,2-Dichloropropane | N.D. | 5.20 | 41.0 | 66.5 | 97.0 | 23.2 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|------------------------|-------|--------|------|-----------|------|-----------|
| cis-1,2-Dichloroethene | N.D. | 5.22 | 61.0 | 167.2 | 98.0 | 67.3 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| Methyl ethyl ketone | N.D. | 5.28 | 72.0 | 21.3 |







| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|
| Bromochloromethane | N.D. | 5.52 | 49.0 | 182.9 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|------------|-------|--------|------|-----------|
| Chloroform | N.D. | 5.65 | 85.0 | 66.0 |




Quantitation Results Report (QT Reviewed)

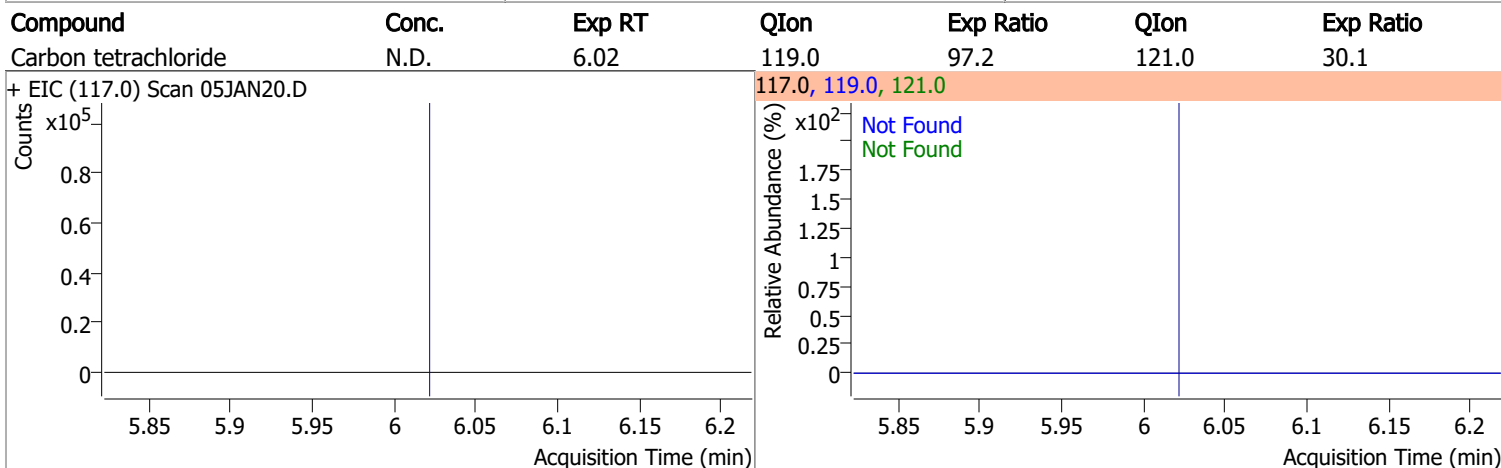


Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 287.1237 | 6.23 | 0.00 | 86001 | 65.0 | 197.6 | 166.5 | 226.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|--------|------|----------|---------|------|--------|-------|-------|
| Benzene | 0.1455 | 6.28 | 0.00 | 427 (m) | 77.0 | 16.0 | 0.0 | 53.5 |







| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,2-Dichloroethane | N.D. | 6.32 | 64.0 | 29.9 | 98.0 | 7.6 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------|-------|--------|-------|-----------|------|-----------|
| Trichloroethene | N.D. | 7.03 | 130.0 | 101.5 | 97.0 | 64.1 |




Quantitation Results Report (QT Reviewed)

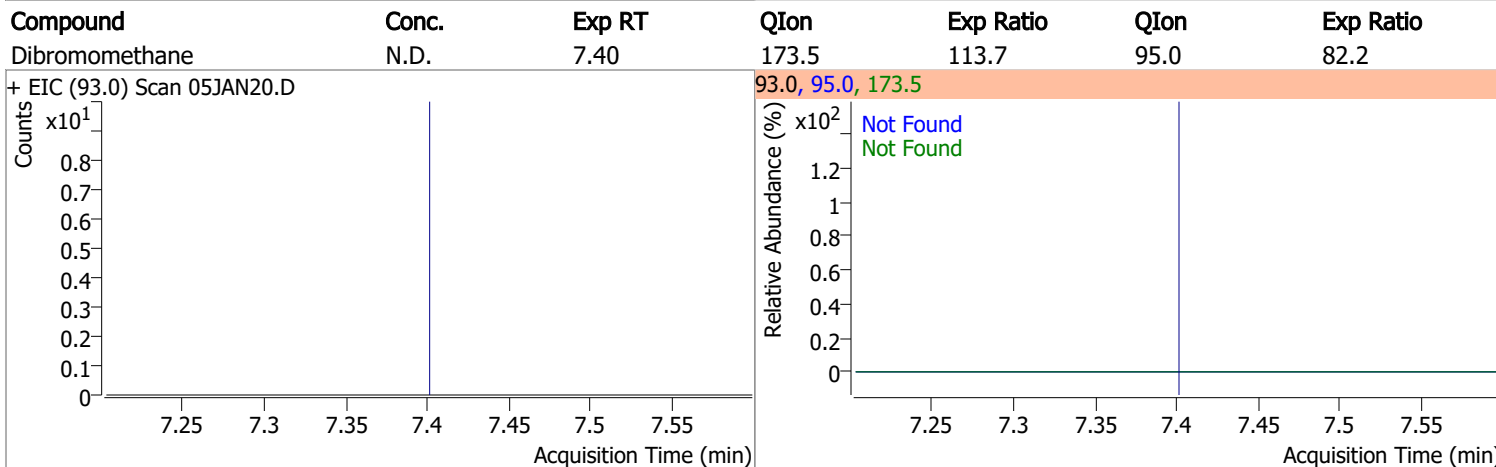


Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 266.9897 | 8.32 | 0.00 | 735346 | 100.0 | 63.6 | 34.4 | 94.4 |
| | | | | | 99.0 | 9.4 | 0.0 | 39.6 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------|-------|--------|------|-----------|
| Toluene | N.D. | 8.39 | 91.0 | 175.8 |











| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,3-Dichloropropene | N.D. | 8.64 | 39.0 | 53.4 | 77.0 | 32.4 |







| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------------|-------|--------|------|-----------|------|-----------|
| 1,1,2-Trichloroethane | N.D. | 8.82 | 97.0 | 114.6 | 85.0 | 67.6 |






Quantitation Results Report (QT Reviewed)
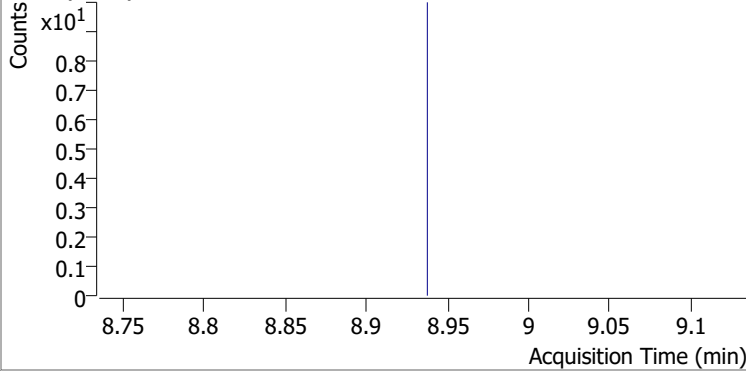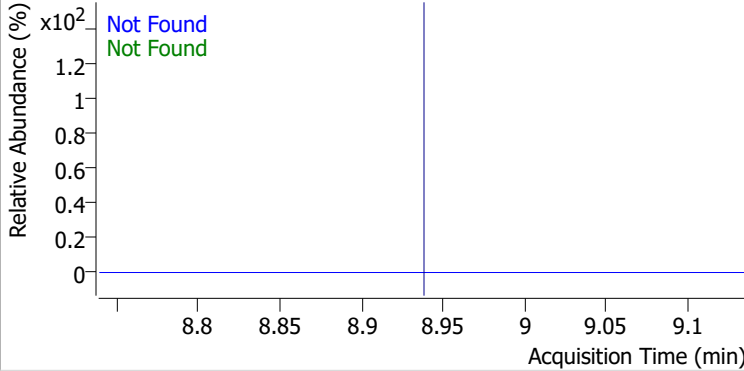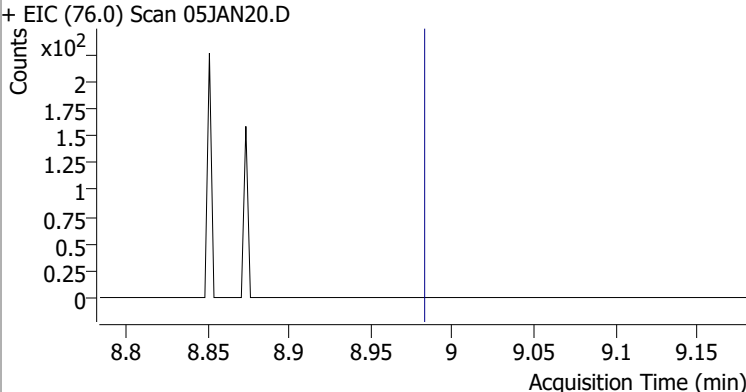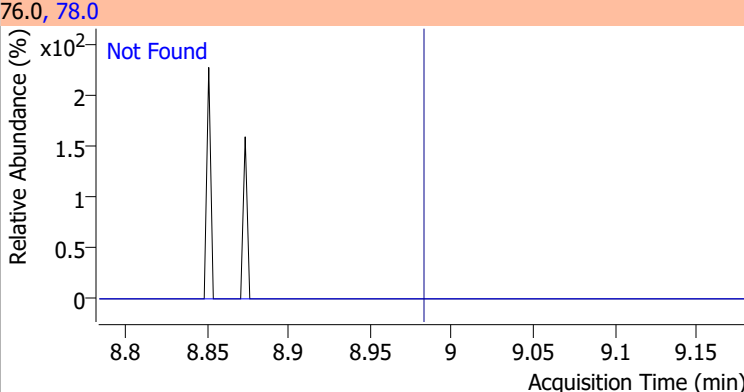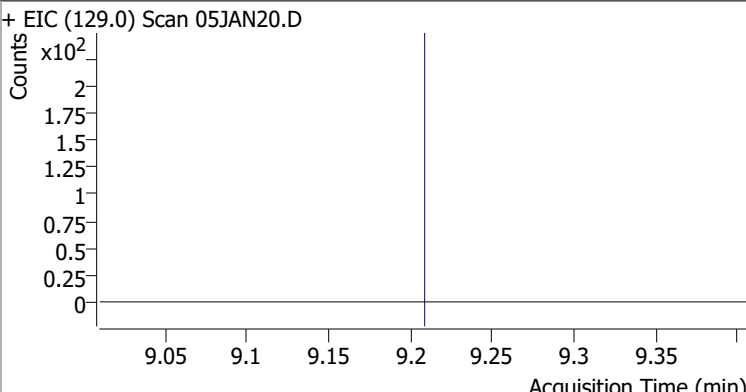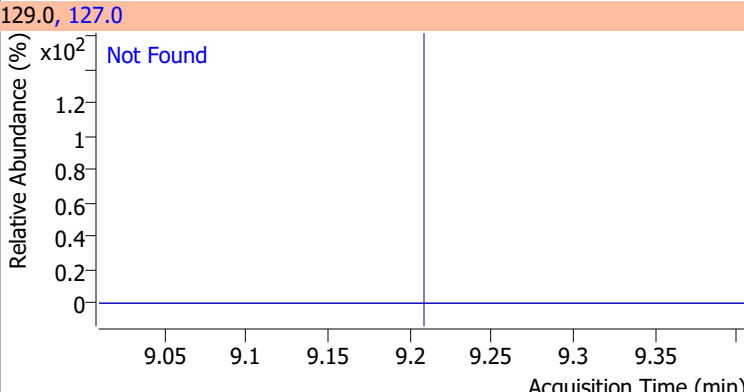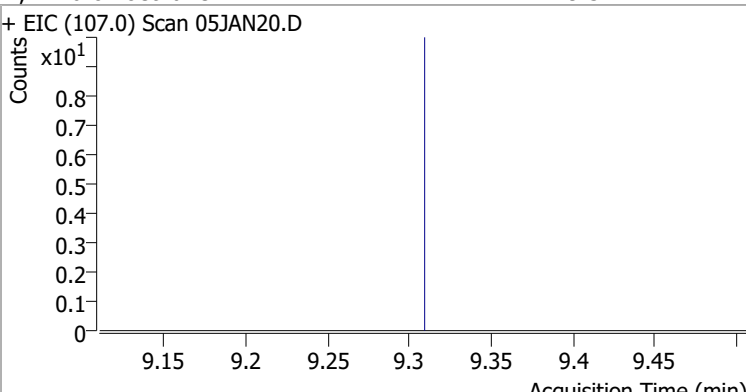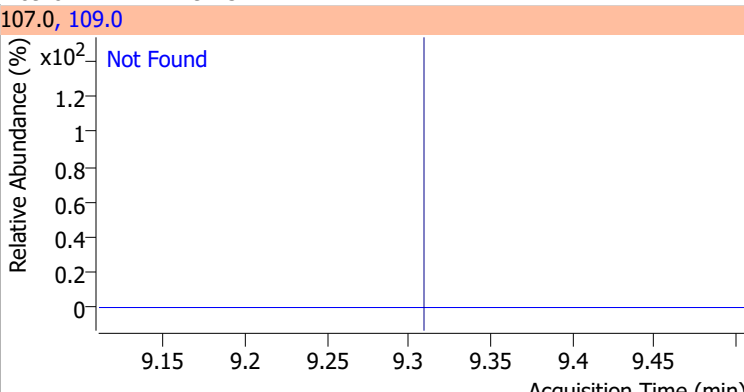
| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--|-------|--------|--|-----------|-------|-----------|
| Tetrachloroethene | N.D. | 8.94 | 165.8 | 128.6 | 129.0 | 91.5 |
| + EIC (163.8) Scan 05JAN20.D ***NO DATA POINTS*** | | | 163.8, 129.0, 165.8 | | | |
|  | | |  | | | |
| 1,3-Dichloropropane | N.D. | 8.98 | 78.0 | 32.9 | | |
| + EIC (76.0) Scan 05JAN20.D | | | 76.0, 78.0 | | | |
|  | | |  | | | |
| Chlorodibromomethane | N.D. | 9.21 | 127.0 | 78.0 | | |
| + EIC (129.0) Scan 05JAN20.D | | | 129.0, 127.0 | | | |
|  | | |  | | | |
| 1,2-Dibromoethane | N.D. | 9.31 | 109.0 | 94.5 | | |
| + EIC (107.0) Scan 05JAN20.D | | | 107.0, 109.0 | | | |
|  | | |  | | | |


Quantitation Results Report (QT Reviewed)

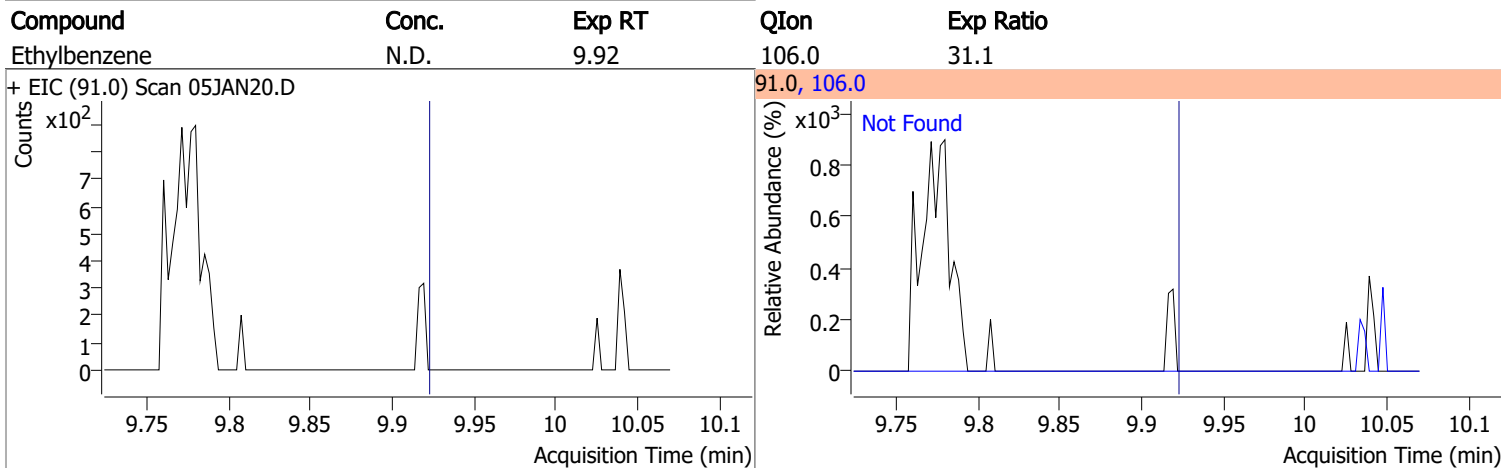









Quantitation Results Report (QT Reviewed)











| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 265.6160 | 10.95 | 0.00 | 212642 | 174.0 | 96.4 | 61.7 | 121.7 |
| | | | | | 176.0 | 93.7 | 60.6 | 120.6 |



Quantitation Results Report (QT Reviewed)

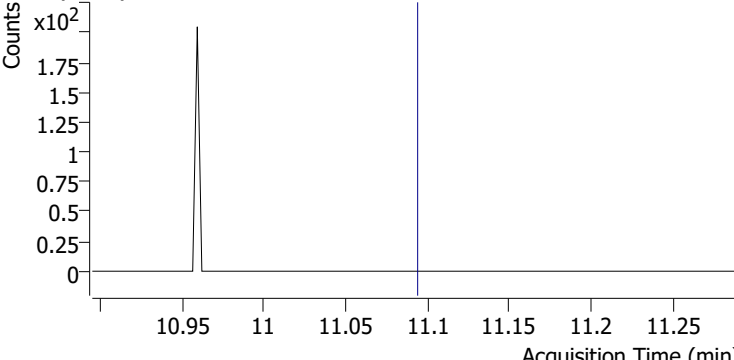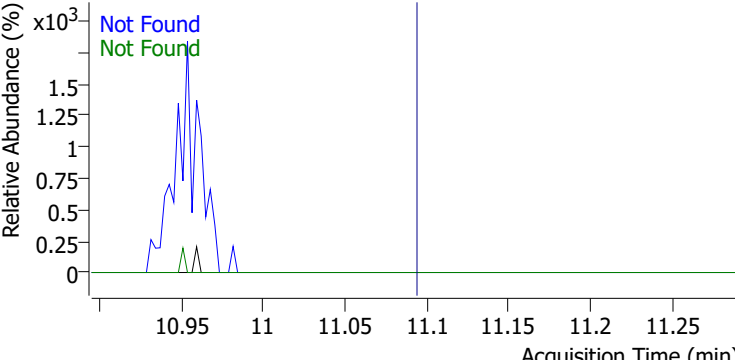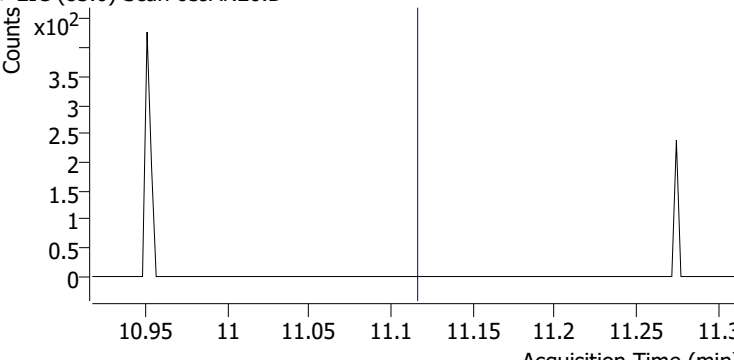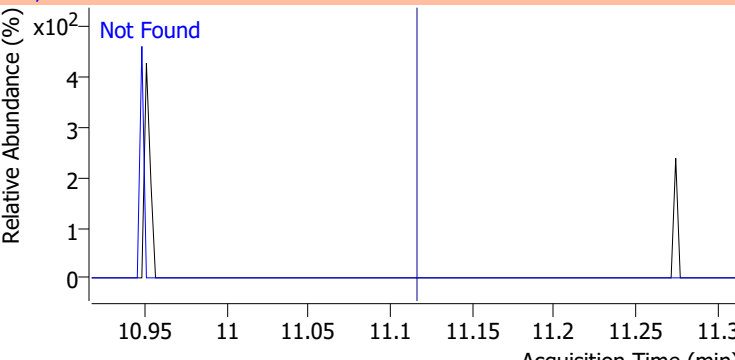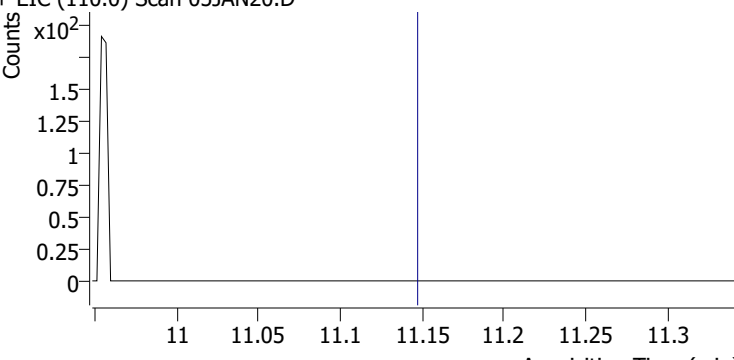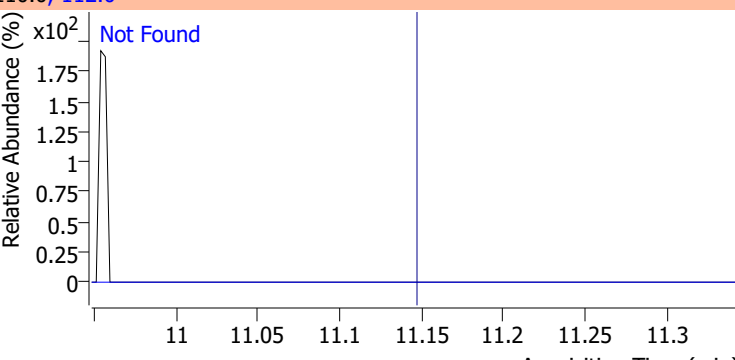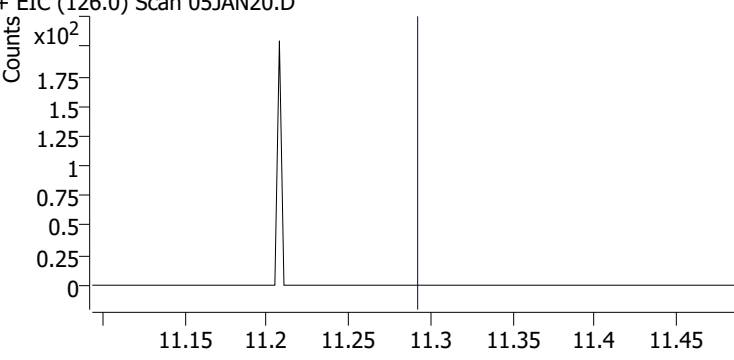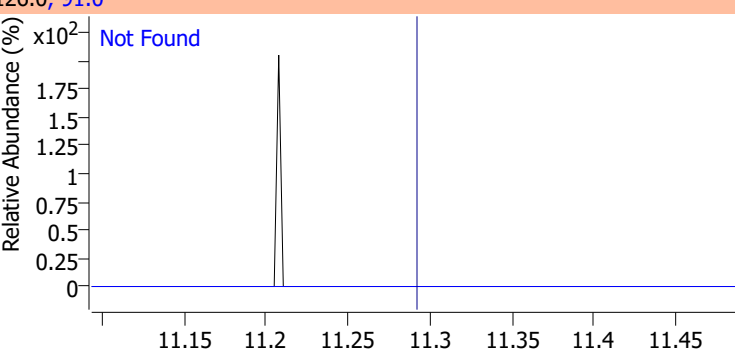
| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--|-------|--------|--|-----------|-------|-----------|
| Bromobenzene | N.D. | 11.09 | 77.0 | 145.7 | 158.0 | 96.5 |
| + EIC (156.0) Scan 05JAN20.D | | | 156.0, 77.0, 158.0 | | | |
|  | | |  | | | |
| 1,1,2,2-Tetrachloroethane | N.D. | 11.12 | 85.0 | 66.2 | | |
| + EIC (83.0) Scan 05JAN20.D | | | 83.0, 85.0 | | | |
|  | | |  | | | |
| 1,2,3-Trichloropropane | N.D. | 11.15 | 112.0 | 63.5 | | |
| + EIC (110.0) Scan 05JAN20.D | | | 110.0, 112.0 | | | |
|  | | |  | | | |
| 2-Chlorotoluene | N.D. | 11.29 | 91.0 | 282.3 | | |
| + EIC (126.0) Scan 05JAN20.D | | | 126.0, 91.0 | | | |
|  | | |  | | | |

Quantitation Results Report (QT Reviewed)
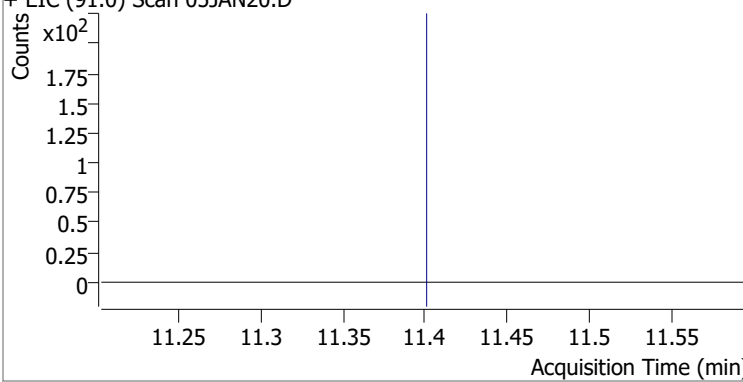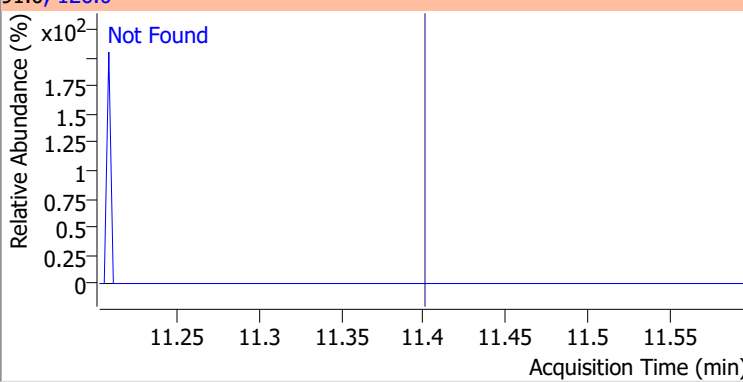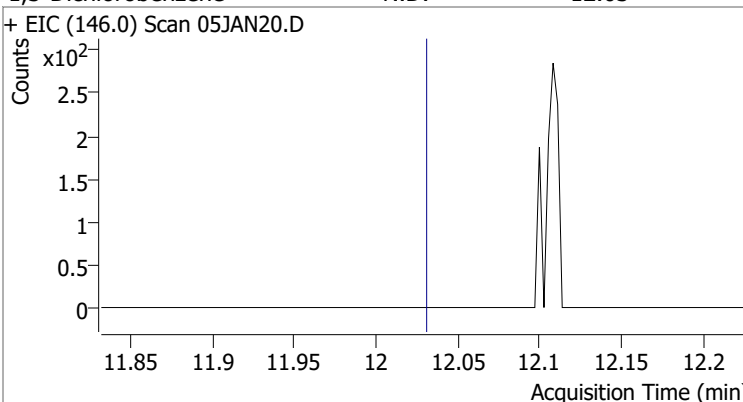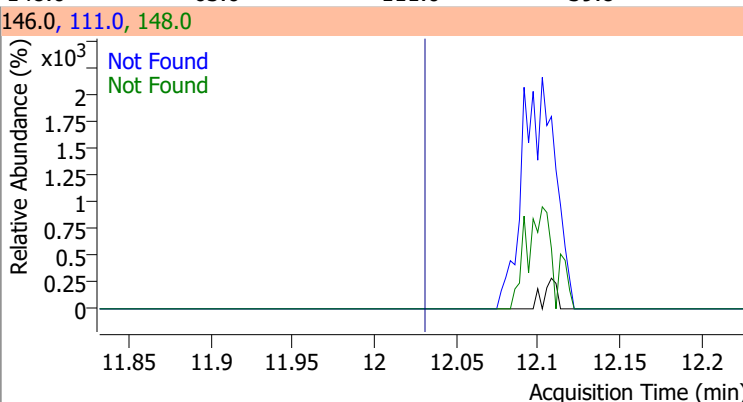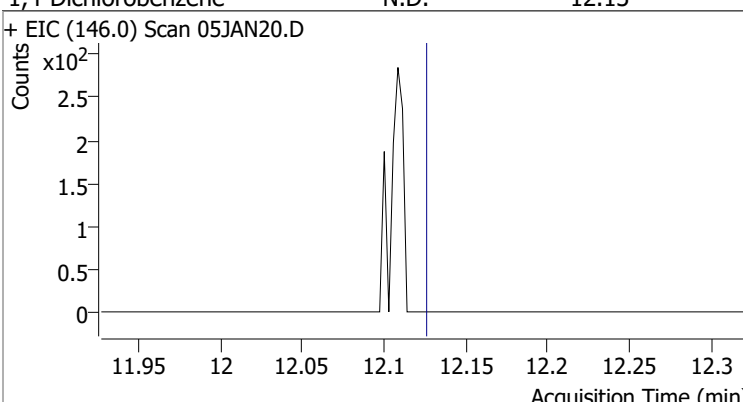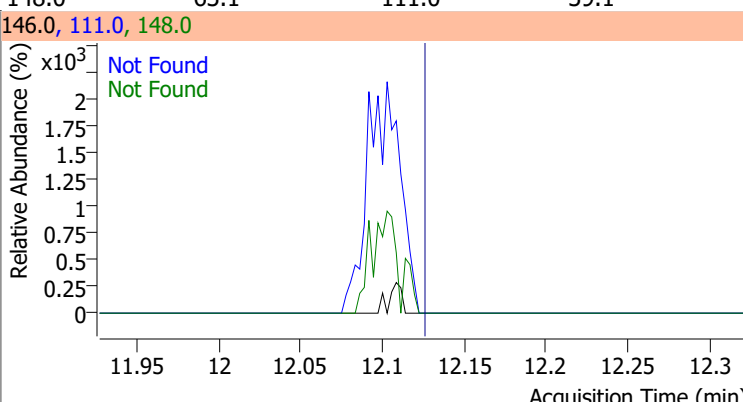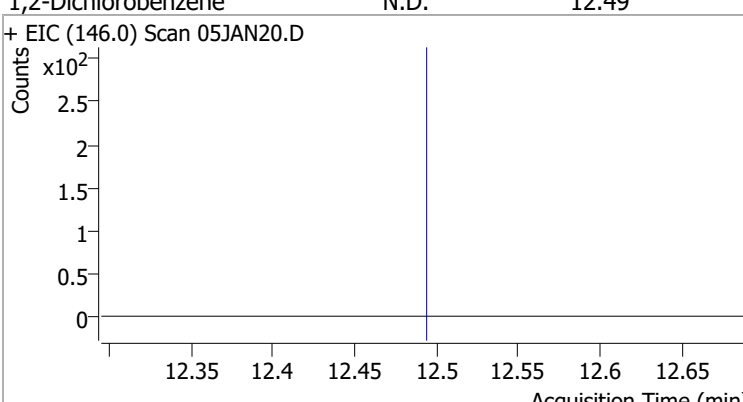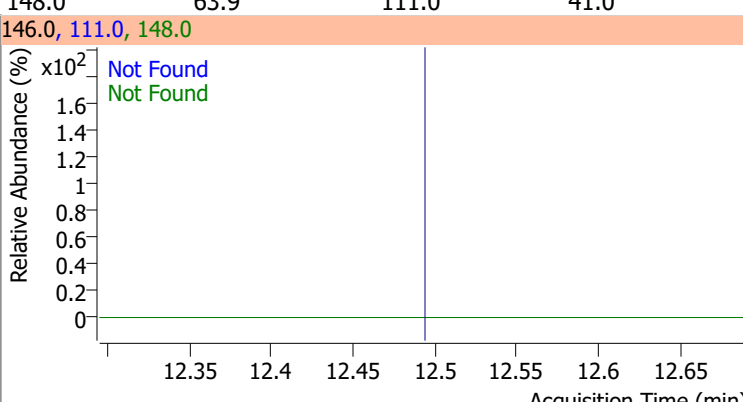
| Compound | Conc. | Exp RT | QIon | Exp Ratio | | |
|--|-------|--------|--|-----------|------|-----------|
| 4-Chlorotoluene | N.D. | 11.40 | 126.0 | 31.7 | | |
| + EIC (91.0) Scan 05JAN20.D | | | 91.0, 126.0 | | | |
|  | | |  | | | |
| 1,3-Dichlorobenzene | N.D. | 12.03 | 148.0 | 63.6 | QIon | Exp Ratio |
| + EIC (146.0) Scan 05JAN20.D | | | 146.0, 111.0, 148.0 | | | |
|  | | |  | | | |
| 1,4-Dichlorobenzene | N.D. | 12.13 | 148.0 | 63.1 | QIon | Exp Ratio |
| + EIC (146.0) Scan 05JAN20.D | | | 146.0, 111.0, 148.0 | | | |
|  | | |  | | | |
| 1,2-Dichlorobenzene | N.D. | 12.49 | 148.0 | 63.9 | QIon | Exp Ratio |
| + EIC (146.0) Scan 05JAN20.D | | | 146.0, 111.0, 148.0 | | | |
|  | | |  | | | |

Quantitation Results Report (QT Reviewed)

| | | | |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File | 05JAN21.D | Operator | MSC |
| Acq. Method | 5975CACQF.M | Acq. Date-Time | 1/5/2022 7:11:33 PM |
| Sample Name | B22010142-001F | Instrument | VOA5975C |
| Vial | 21 | Multiplier | 1.00 |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m | Comment | |
| Tune File | BFB_Atune3.u | Tune Date | 10/11/2021 4:02:00 PM |
| Batch Name | VG010522_8260B.batch.bin | Last Calib Update | 2/28/2022 2:48:47 PM |
| Ref Library | \\MASSHUNTER\Org\Library\NIST129K.l | | |



| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|----------|----|------|-------|-------|-------|----------|
|----------|----|------|-------|-------|-------|----------|

Internal Standards

| | | | | | | |
|--------------------------|--------|-------|--------|----------|----|--------|
| M Fluorobenzene | 6.621 | 96.0 | 727110 | 250.0000 | ng | -0.003 |
| M Chlorobenzene-d5 | 9.774 | 82.0 | 284647 | 250.0000 | ng | 0.003 |
| M 1,4-Dichlorobenzene-d4 | 12.100 | 152.0 | 215573 | 250.0000 | ng | 0.000 |

System Monitoring Compounds

| | | | | | | |
|-------------------------|----------------------|-------|--------|--------------------|----|--------|
| S Dibromofluoromethane | 5.845 | 113.0 | 193407 | 282.3413 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 80.0 - 119.0% | | | Recovery = 112.94% | | |
| S 1,2-Dichloroethane-d4 | 6.230 | 67.0 | 87221 | 294.7895 | ng | -0.003 |
| Spiked Amount: 250.000 | Range: 81.0 - 118.0% | | | Recovery = 117.92% | | |
| S Toluene-d8 | 8.319 | 98.0 | 729970 | 266.1207 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 89.0 - 112.0% | | | Recovery = 106.45% | | |
| S p-Bromofluorobenzene | 10.954 | 95.0 | 214122 | 271.1248 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 85.0 - 114.0% | | | Recovery = 108.45% | | |

Target Compounds

| Compound | RT | QIon | Resp. | Conc. | Units | QValue |
|----------------------------------|-------|------|-------|--------|-------|--------|
| T Dichlorodifluoromethane | 0.000 | | 0 | N.D. | | |
| T Chloromethane | 1.406 | 50.0 | 1801 | 1.5575 | ng m | 87 |
| T Vinyl chloride | 0.000 | | 0 | N.D. | | |
| T Bromomethane | 0.000 | | 0 | N.D. | | |
| T Chloroethane | 0.000 | | 0 | N.D. | | |
| T Trichlorofluoromethane | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methylene chloride | 0.000 | | 0 | N.D. | | |
| T trans-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methyl tert-butyl ether (MTBE) | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloroethane | 0.000 | | 0 | N.D. | | |
| T 2,2-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T cis-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methyl ethyl ketone | 0.000 | | 0 | N.D. | | |
| T Bromochloromethane | 0.000 | | 0 | N.D. | | |
| T Chloroform | 0.000 | | 0 | N.D. | | |


Quantitation Results Report (QT Reviewed)

| Compound | RT | QIon | Resp. | Conc. | Units | | Dev(Min) |
|-----------------------------|-------|------|-------|--------|-------|---|----------|
| T 1,1,1-Trichloroethane | 0.000 | | 0 | N.D. | | | |
| T Carbon tetrachloride | 0.000 | | 0 | N.D. | | | |
| T 1,1-Dichloropropene | 0.000 | | 0 | N.D. | | | |
| T Benzene | 6.278 | 78.0 | 280 | 0.0968 | ng | m | 71 |
| T 1,2-Dichloroethane | 0.000 | | 0 | N.D. | | | |
| T Trichloroethene | 0.000 | | 0 | N.D. | | | |
| T 1,2-Dichloropropane | 0.000 | | 0 | N.D. | | | |
| T Dibromomethane | 0.000 | | 0 | N.D. | | | |
| T Bromodichloromethane | 0.000 | | 0 | N.D. | | | |
| T cis-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | | |
| T Toluene | 8.389 | 92.0 | 2211 | 1.1933 | ng | | 88 |
| T trans-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | | |
| T 1,1,2-Trichloroethane | 0.000 | | 0 | N.D. | | | |
| T Tetrachloroethene | 0.000 | | 0 | N.D. | | | |
| T 1,3-Dichloropropane | 0.000 | | 0 | N.D. | | | |
| T Chlorodibromomethane | 0.000 | | 0 | N.D. | | | |
| T 1,2-Dibromoethane | 0.000 | | 0 | N.D. | | | |
| T Chlorobenzene | 0.000 | | 0 | N.D. | | | |
| T 1,1,1,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | | |
| T Ethylbenzene | 0.000 | | 0 | N.D. | | | |
| T m+p-Xylenes | 0.000 | | 0 | N.D. | | | |
| T o-Xylene | 0.000 | | 0 | N.D. | | | |
| T Styrene | 0.000 | | 0 | N.D. | | | |
| T Bromoform | 0.000 | | 0 | N.D. | | | |
| T Bromobenzene | 0.000 | | 0 | N.D. | | | |
| T 1,1,2,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | | |
| T 1,2,3-Trichloropropane | 0.000 | | 0 | N.D. | | | |
| T 2-Chlorotoluene | 0.000 | | 0 | N.D. | | | |
| T 4-Chlorotoluene | 0.000 | | 0 | N.D. | | | |
| T 1,3-Dichlorobenzene | 0.000 | | 0 | N.D. | | | |
| T 1,4-Dichlorobenzene | 0.000 | | 0 | N.D. | | | |
| T 1,2-Dichlorobenzene | 0.000 | | 0 | N.D. | | | |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|-------------------------|-------|--------|------|-----------|
| Dichlorodifluoromethane | N.D. | 1.24 | 87.0 | 32.3 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------|--------|------|----------|----------|------|--------|-------|-------|
| Chloromethane | 1.5575 | 1.41 | 0.00 | 1801 (m) | 52.0 | 24.9 | 2.1 | 62.1 |











| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------------|-------|--------|------|-----------|
| Vinyl chloride | N.D. | 1.50 | 64.0 | 29.9 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------|-------|--------|------|-----------|
| Bromomethane | N.D. | 1.80 | 94.0 | 104.6 |




Quantitation Results Report (QT Reviewed)

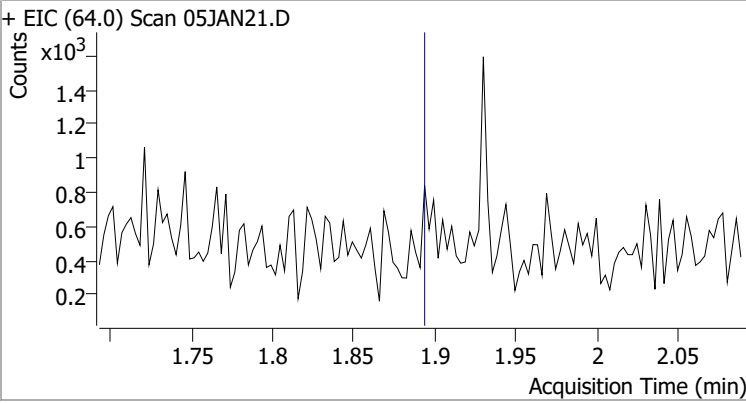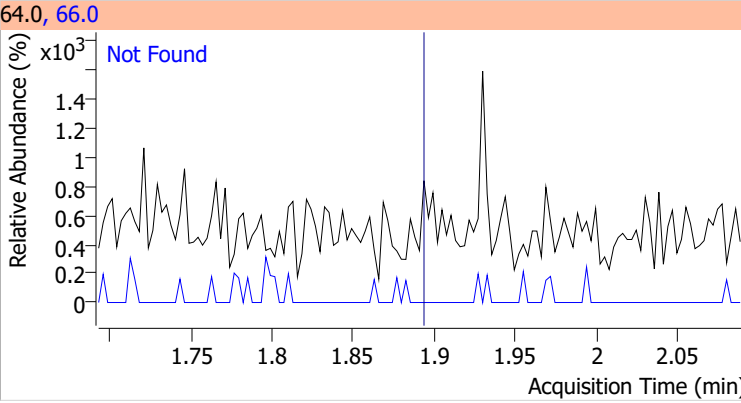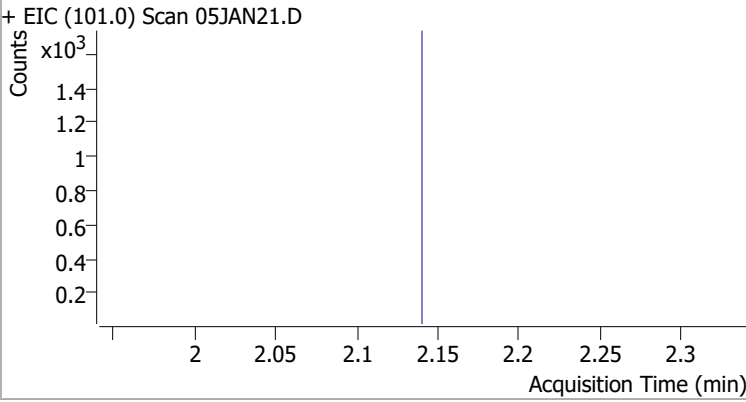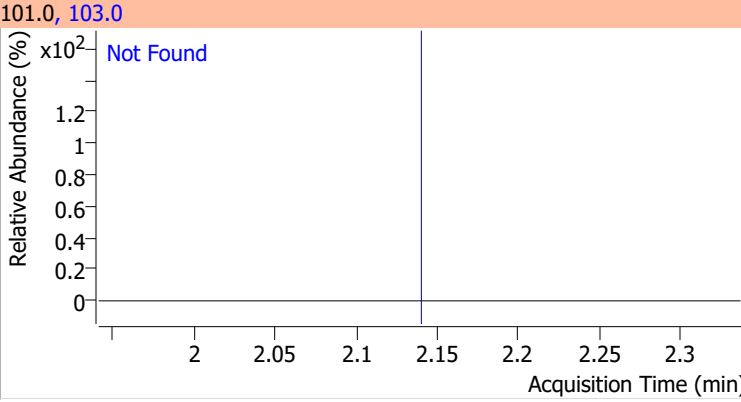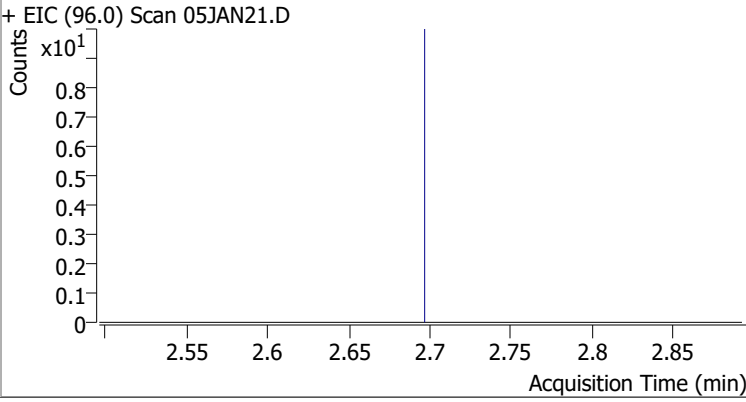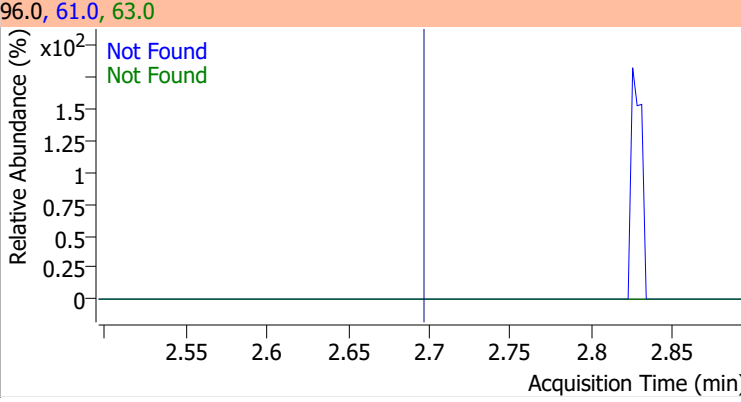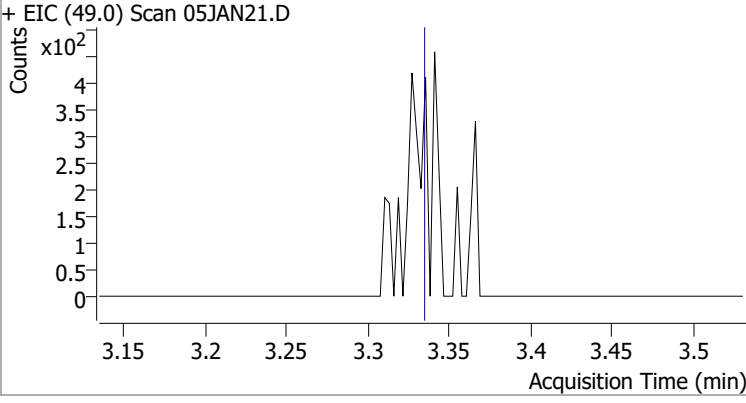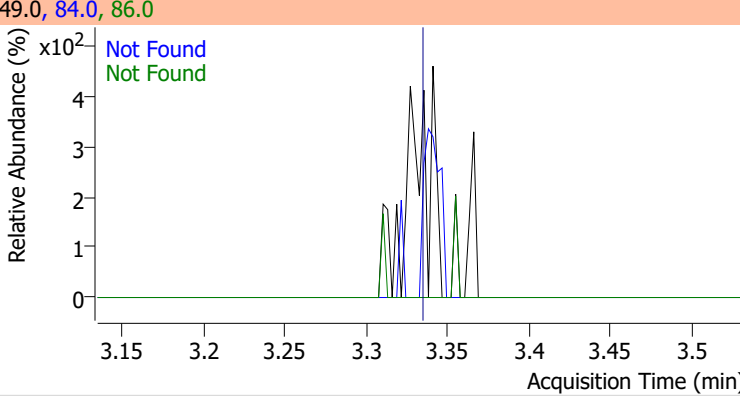
| Compound | Conc. | Exp RT | QIon | Exp Ratio | | |
|--|-------|--------|--|-----------|------|-----------|
| Chloroethane | N.D. | 1.89 | 66.0 | 30.1 | | |
| + EIC (64.0) Scan 05JAN21.D | | | 64.0, 66.0 | | | |
|  | | |  | | | |
| Trichlorofluoromethane | N.D. | 2.14 | 103.0 | 64.2 | | |
| + EIC (101.0) Scan 05JAN21.D | | | 101.0, 103.0 | | | |
|  | | |  | | | |
| 1,1-Dichloroethene | N.D. | 2.70 | 61.0 | 180.3 | QIon | Exp Ratio |
| | | | 63.0 | 56.7 | | |
| + EIC (96.0) Scan 05JAN21.D | | | 96.0, 61.0, 63.0 | | | |
|  | | |  | | | |
| Methylene chloride | N.D. | 3.34 | 84.0 | 66.9 | QIon | Exp Ratio |
| | | | 86.0 | 44.3 | | |
| + EIC (49.0) Scan 05JAN21.D | | | 49.0, 84.0, 86.0 | | | |
|  | | |  | | | |

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,2-Dichloroethene | N.D. | 3.72 | 61.0 | 153.9 | 98.0 | 65.7 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------------------|-------|--------|------|-----------|
| Methyl tert-butyl ether (MTBE) | N.D. | 3.75 | 57.0 | 24.6 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethane | N.D. | 4.38 | 65.0 | 32.1 | 83.0 | 13.7 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|------|-----------|
| 2,2-Dichloropropane | N.D. | 5.20 | 41.0 | 66.5 | 97.0 | 23.2 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|------------------------|-------|--------|------|-----------|------|-----------|
| cis-1,2-Dichloroethene | N.D. | 5.22 | 61.0 | 167.2 | 98.0 | 67.3 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| Methyl ethyl ketone | N.D. | 5.28 | 72.0 | 21.3 |







| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|
| Bromochloromethane | N.D. | 5.52 | 49.0 | 182.9 |







| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|------------|-------|--------|------|-----------|
| Chloroform | N.D. | 5.65 | 85.0 | 66.0 |







Quantitation Results Report (QT Reviewed)

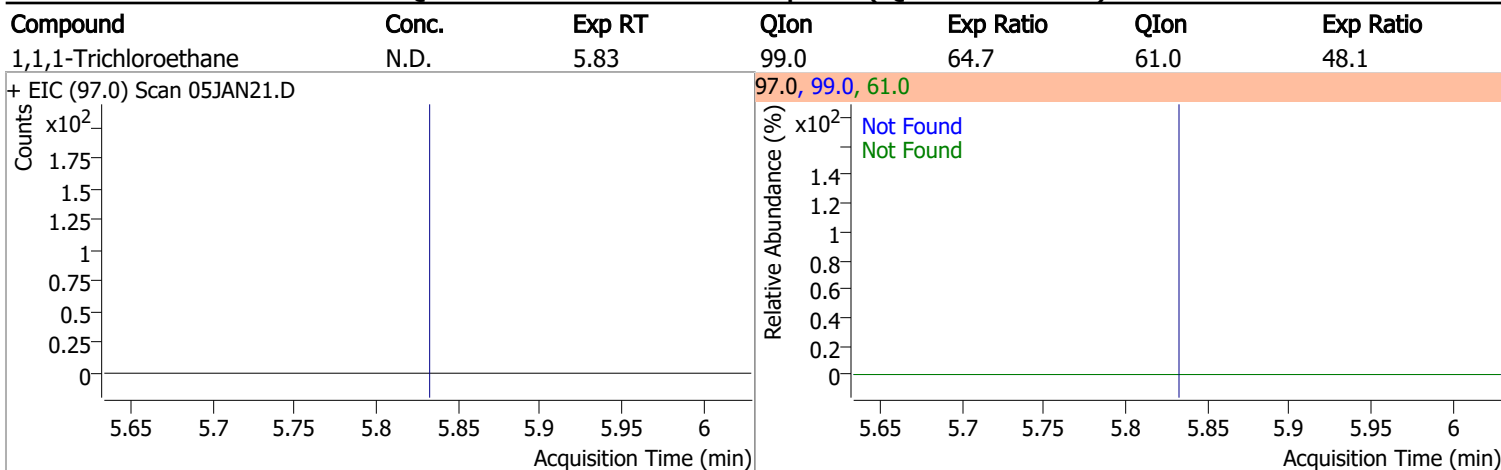

Quantitation Results Report (QT Reviewed)

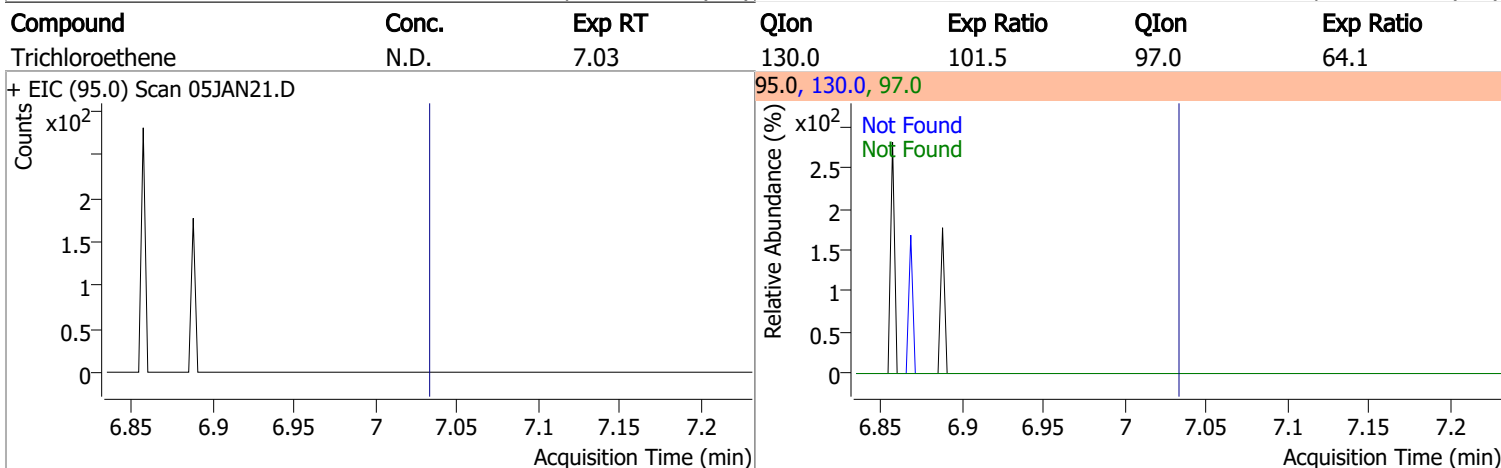


Quantitation Results Report (QT Reviewed)

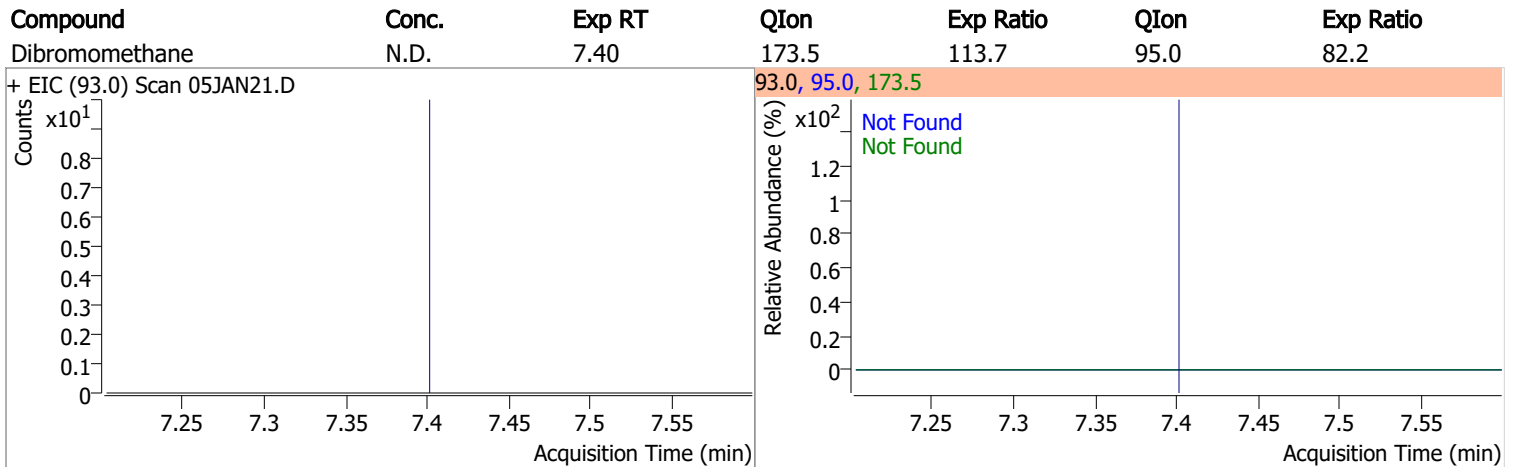


Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 266.1207 | 8.32 | 0.00 | 729970 | 100.0 | 64.1 | 34.4 | 94.4 |
| | | | | | 99.0 | 9.7 | 0.0 | 39.6 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|--------|------|----------|-------|------|--------|-------|-------|
| Toluene | 1.1933 | 8.39 | 0.00 | 2211 | 91.0 | 192.0 | 145.8 | 205.8 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,3-Dichloropropene | N.D. | 8.64 | 39.0 | 53.4 | 77.0 | 32.4 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------------|-------|--------|------|-----------|------|-----------|
| 1,1,2-Trichloroethane | N.D. | 8.82 | 97.0 | 114.6 | 85.0 | 67.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-------------------|-------|--------|-------|-----------|-------|-----------|
| Tetrachloroethene | N.D. | 8.94 | 165.8 | 128.6 | 129.0 | 91.5 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| 1,3-Dichloropropane | N.D. | 8.98 | 78.0 | 32.9 |











| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------------------|-------|--------|-------|-----------|
| Chlorodibromomethane | N.D. | 9.21 | 127.0 | 78.0 |






| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|-------------------|-------|--------|-------|-----------|
| 1,2-Dibromoethane | N.D. | 9.31 | 109.0 | 94.5 |




Quantitation Results Report (QT Reviewed)
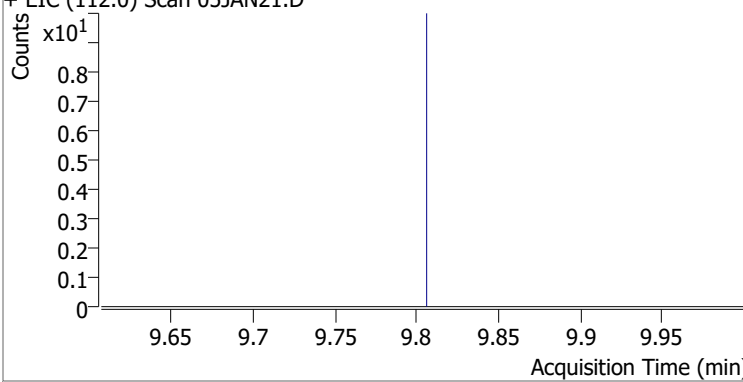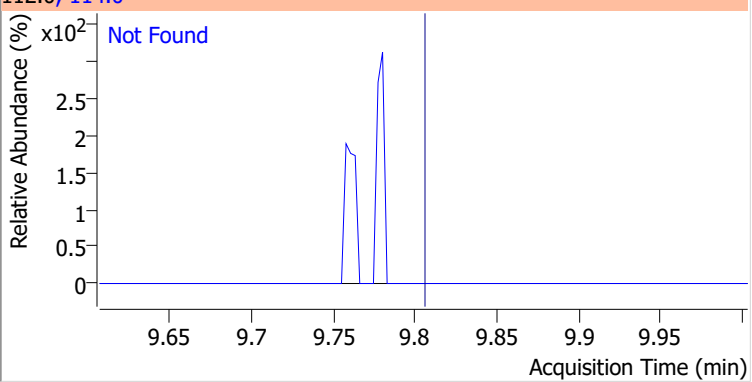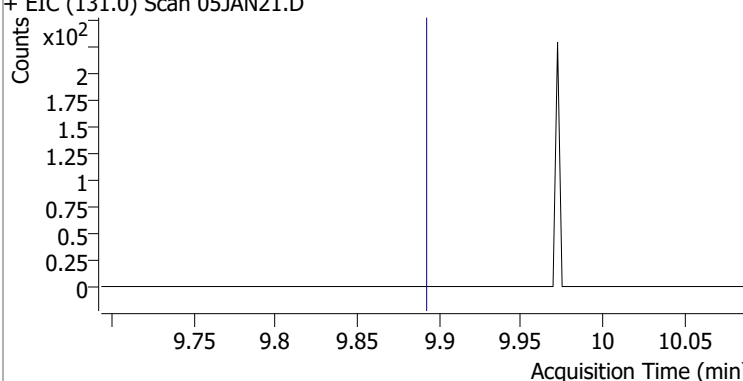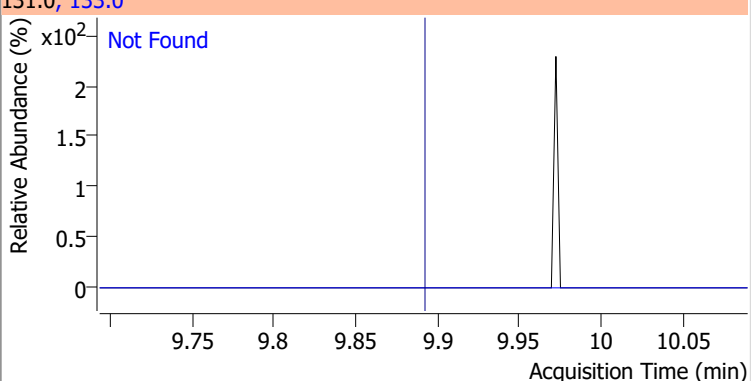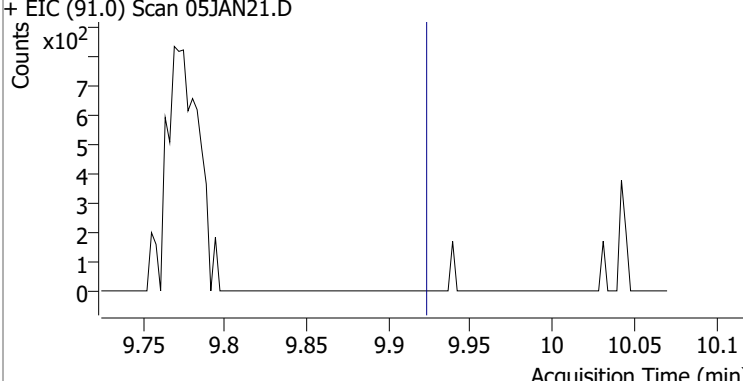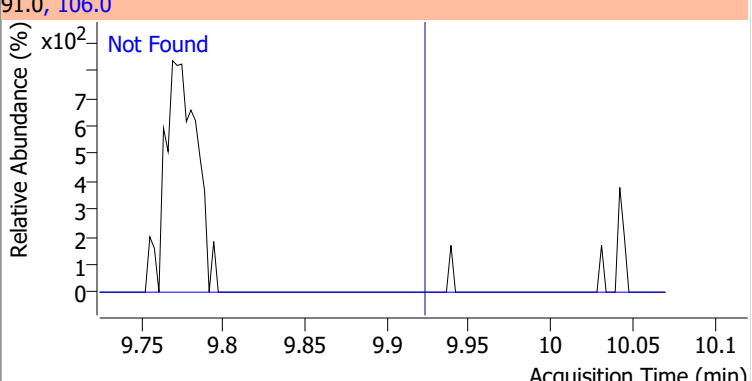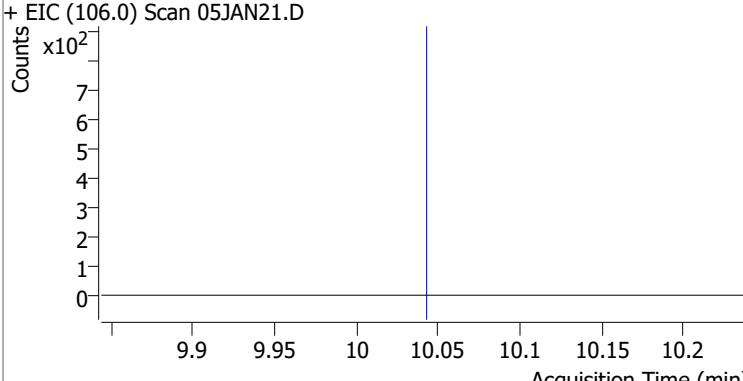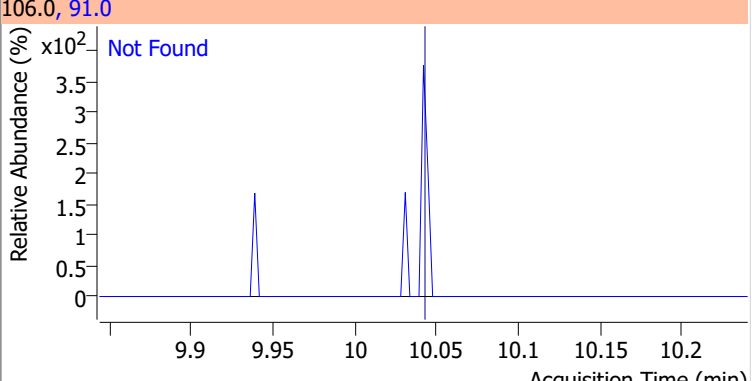
| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--|-------|--------|--|-----------|
| Chlorobenzene | N.D. | 9.80 | 114.0 | 32.1 |
| + EIC (112.0) Scan 05JAN21.D | | | 112.0, 114.0 | |
|  | | |  | |
| 1,1,1,2-Tetrachloroethane | N.D. | 9.89 | 133.0 | 98.6 |
| + EIC (131.0) Scan 05JAN21.D | | | 131.0, 133.0 | |
|  | | |  | |
| Ethylbenzene | N.D. | 9.92 | 106.0 | 31.1 |
| + EIC (91.0) Scan 05JAN21.D | | | 91.0, 106.0 | |
|  | | |  | |
| m+p-Xylenes | N.D. | 10.04 | 91.0 | 201.4 |
| + EIC (106.0) Scan 05JAN21.D | | | 106.0, 91.0 | |
|  | | |  | |









Quantitation Results Report (QT Reviewed)

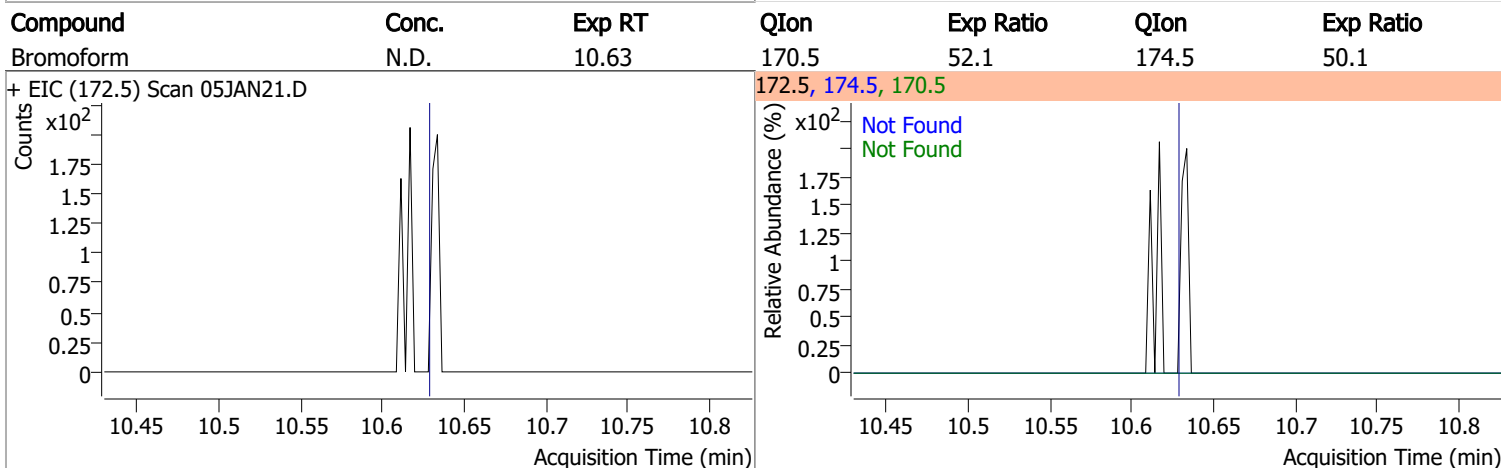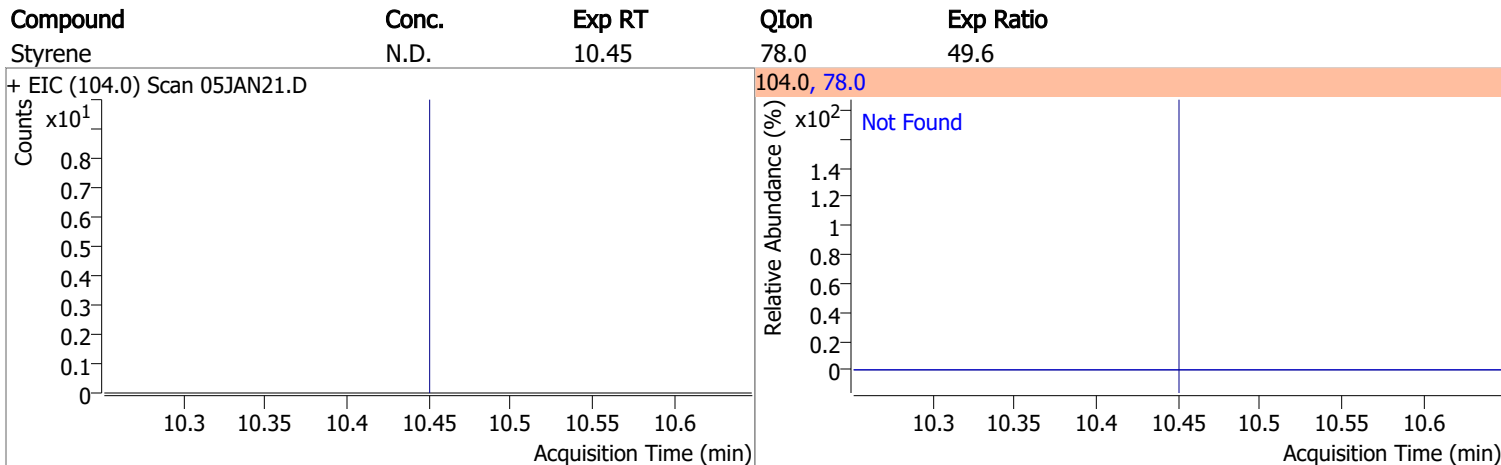









| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 271.1248 | 10.95 | 0.00 | 214122 | 174.0 | 93.3 | 61.7 | 121.7 |
| | | | | | 176.0 | 91.6 | 60.6 | 120.6 |



Quantitation Results Report (QT Reviewed)

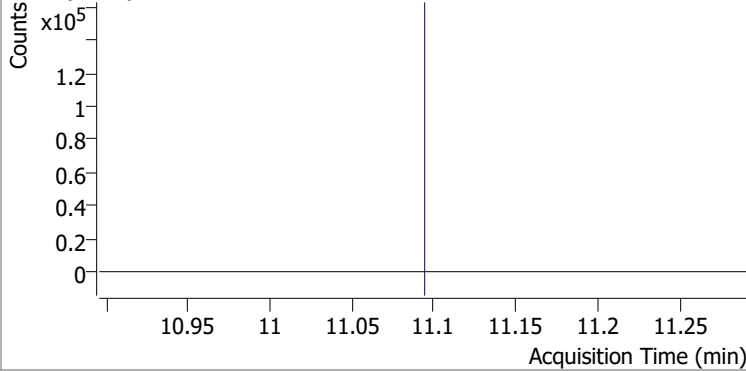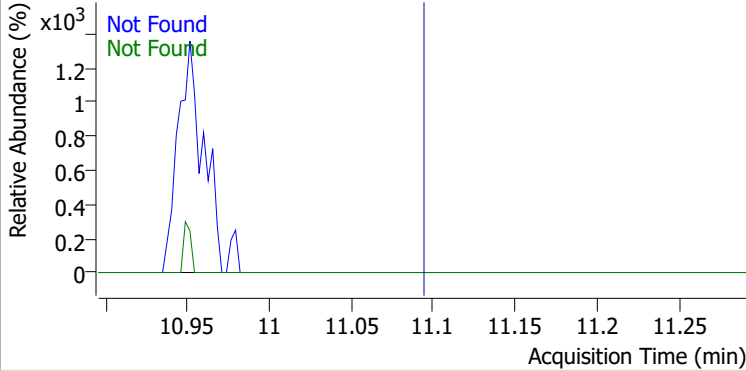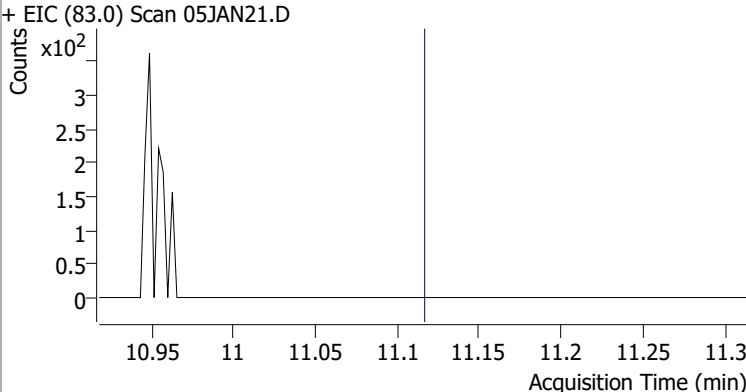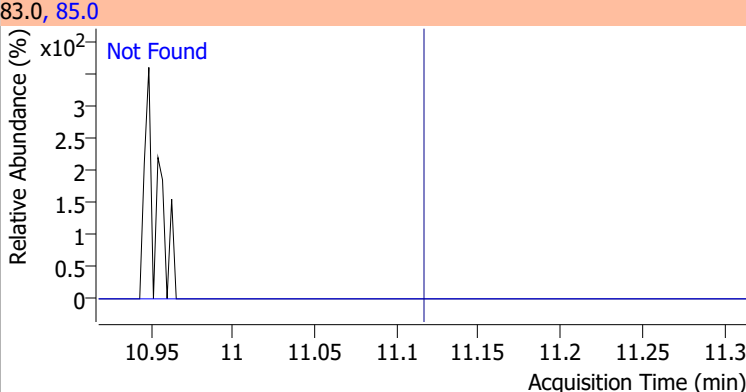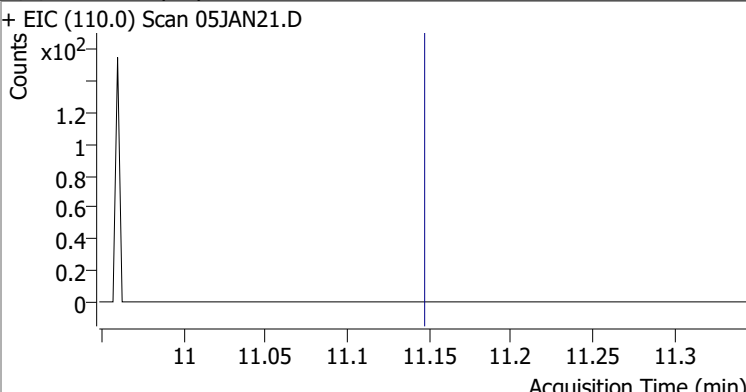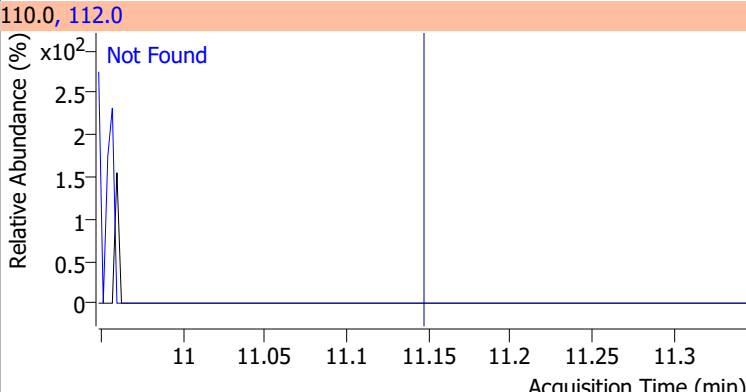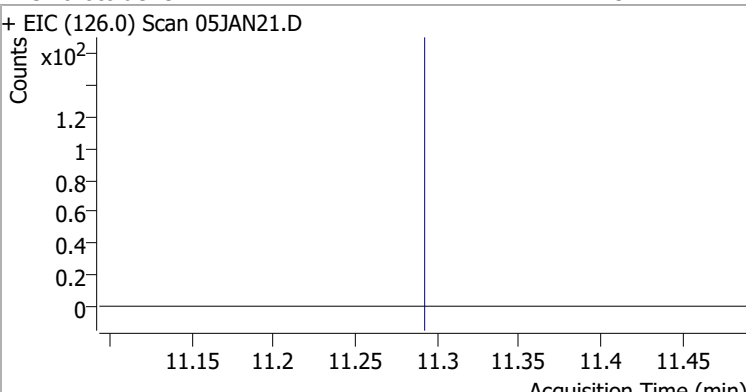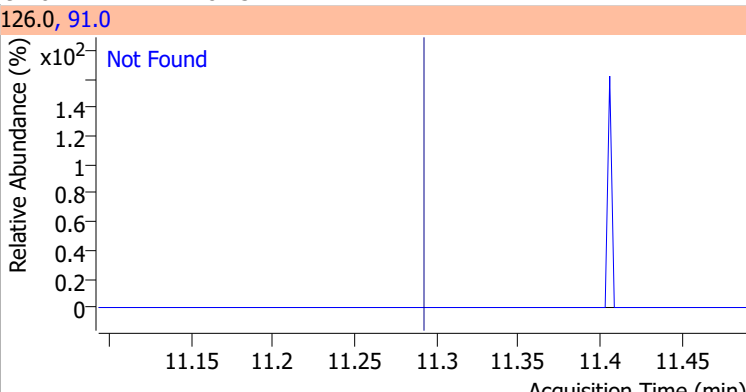
| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--|-------|--------|--|-----------|-------|-----------|
| Bromobenzene | N.D. | 11.09 | 77.0 | 145.7 | 158.0 | 96.5 |
| + EIC (156.0) Scan 05JAN21.D | | | 156.0, 77.0, 158.0 | | | |
|  | | |  | | | |
| 1,1,2,2-Tetrachloroethane | N.D. | 11.12 | 85.0 | 66.2 | | |
| + EIC (83.0) Scan 05JAN21.D | | | 83.0, 85.0 | | | |
|  | | |  | | | |
| 1,2,3-Trichloropropane | N.D. | 11.15 | 112.0 | 63.5 | | |
| + EIC (110.0) Scan 05JAN21.D | | | 110.0, 112.0 | | | |
|  | | |  | | | |
| 2-Chlorotoluene | N.D. | 11.29 | 91.0 | 282.3 | | |
| + EIC (126.0) Scan 05JAN21.D | | | 126.0, 91.0 | | | |
|  | | |  | | | |

Quantitation Results Report (QT Reviewed)
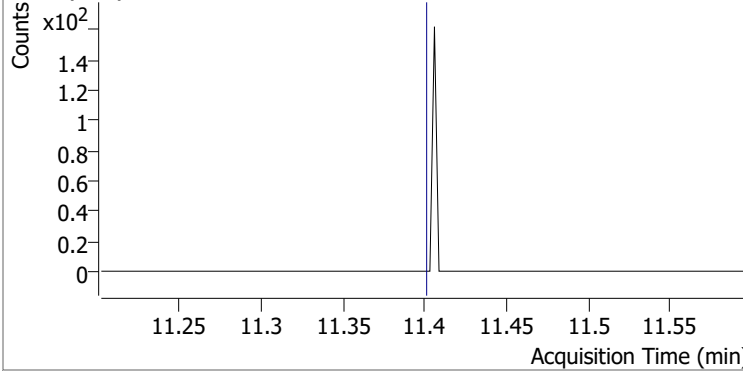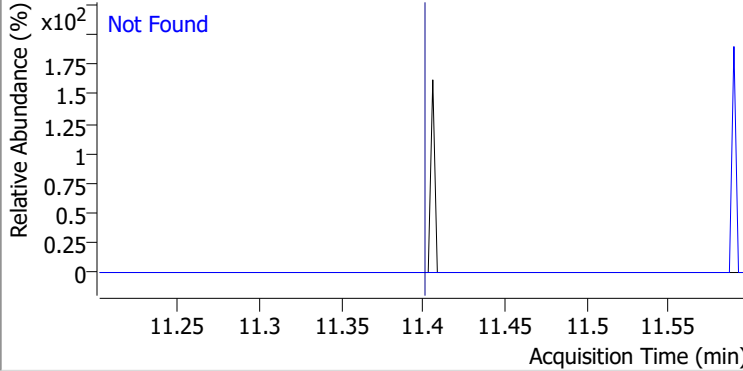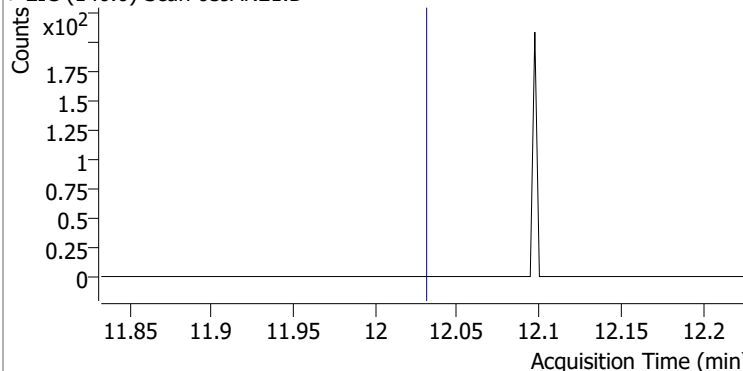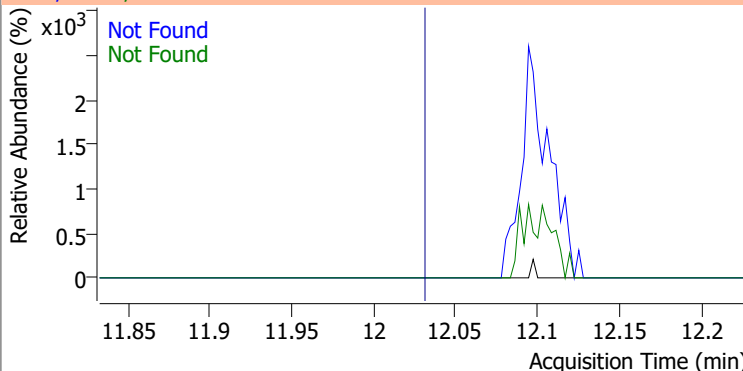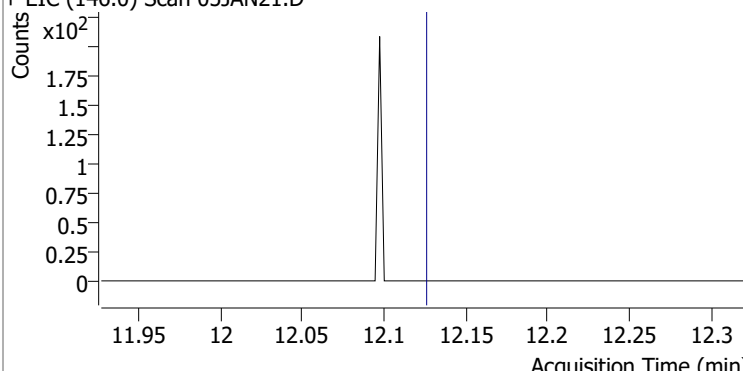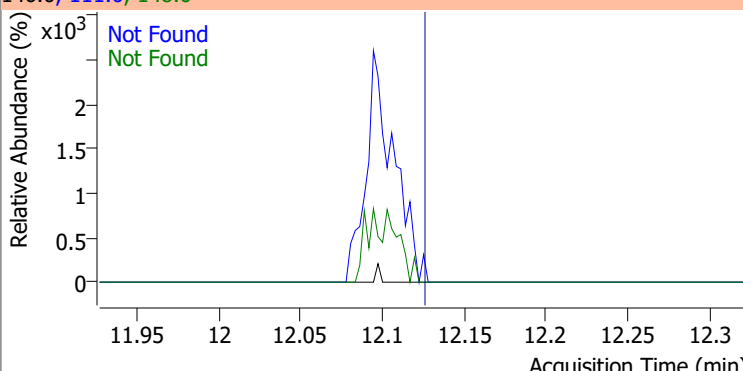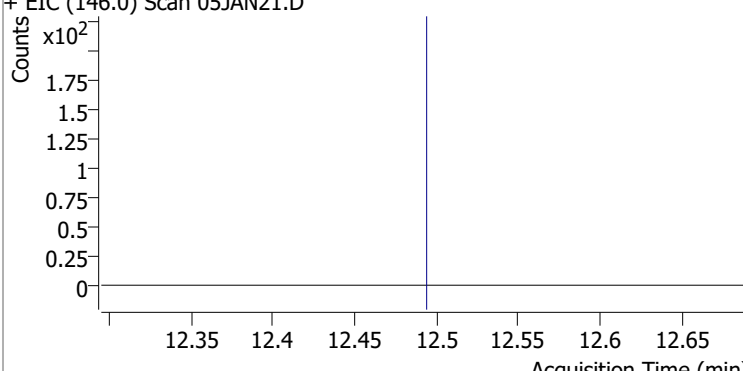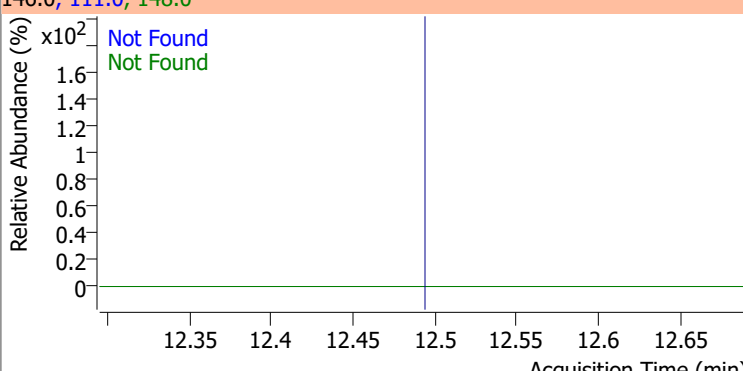
| Compound | Conc. | Exp RT | QIon | Exp Ratio | | |
|--|-------|--------|--|-----------|------|-----------|
| 4-Chlorotoluene | N.D. | 11.40 | 126.0 | 31.7 | | |
| + EIC (91.0) Scan 05JAN21.D | | | 91.0, 126.0 | | | |
|  | | |  | | | |
| 1,3-Dichlorobenzene | N.D. | 12.03 | 148.0 | 63.6 | QIon | Exp Ratio |
| + EIC (146.0) Scan 05JAN21.D | | | 146.0, 111.0, 148.0 | | | |
|  | | |  | | | |
| 1,4-Dichlorobenzene | N.D. | 12.13 | 148.0 | 63.1 | QIon | Exp Ratio |
| + EIC (146.0) Scan 05JAN21.D | | | 146.0, 111.0, 148.0 | | | |
|  | | |  | | | |
| 1,2-Dichlorobenzene | N.D. | 12.49 | 148.0 | 63.9 | QIon | Exp Ratio |
| + EIC (146.0) Scan 05JAN21.D | | | 146.0, 111.0, 148.0 | | | |
|  | | |  | | | |

Quantitation Results Report (QT Reviewed)

| | | | |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File | 05JAN22.D | Operator | MSC |
| Acq. Method | 5975CACQF.M | Acq. Date-Time | 1/5/2022 7:38:52 PM |
| Sample Name | B22010143-001F | Instrument | VOA5975C |
| Vial | 22 | Multiplier | 1.00 |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m | Comment | |
| Tune File | BFB_Atune3.u | Tune Date | 10/11/2021 4:02:00 PM |
| Batch Name | VG010522_8260B.batch.bin | Last Calib Update | 2/28/2022 2:48:47 PM |
| Ref Library | \\MASSHUNTER\Org\Library\NIST129K.I | | |







| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|--------------------|-------|----------|
| Internal Standards | | | | | | |
| M Fluorobenzene | 6.620 | 96.0 | 719788 | 250.0000 | ng | -0.003 |
| M Chlorobenzene-d5 | 9.772 | 82.0 | 282094 | 250.0000 | ng | 0.000 |
| M 1,4-Dichlorobenzene-d4 | 12.100 | 152.0 | 209754 | 250.0000 | ng | 0.000 |
| System Monitoring Compounds | | | | | | |
| S Dibromofluoromethane | 5.848 | 113.0 | 191734 | 282.7463 | ng | 0.003 |
| Spiked Amount: 250.000 | Range: 80.0 - 119.0% | | | Recovery = 113.10% | | |
| S 1,2-Dichloroethane-d4 | 6.233 | 67.0 | 84285 | 287.7642 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 81.0 - 118.0% | | | Recovery = 115.11% | | |
| S Toluene-d8 | 8.319 | 98.0 | 719407 | 264.6434 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 89.0 - 112.0% | | | Recovery = 105.86% | | |
| S p-Bromofluorobenzene | 10.951 | 95.0 | 207569 | 270.1186 | ng | -0.003 |
| Spiked Amount: 250.000 | Range: 85.0 - 114.0% | | | Recovery = 108.05% | | |
| Target Compounds | | | | | | |
| T Dichlorodifluoromethane | 0.000 | | 0 | N.D. | | |
| T Chloromethane | 1.411 | 50.0 | 3703 | 3.2345 | ng | 89 |
| T Vinyl chloride | 0.000 | | 0 | N.D. | | |
| T Bromomethane | 0.000 | | 0 | N.D. | | |
| T Chloroethane | 1.899 | 64.0 | 1664 | 3.2620 | ng | m 91 |
| T Trichlorofluoromethane | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methylene chloride | 3.330 | 49.0 | 1094 | 1.0233 | ng | m 85 |
| T trans-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methyl tert-butyl ether (MTBE) | 0.000 | | 0 | N.D. | | |
| T 1,1-Dichloroethane | 0.000 | | 0 | N.D. | | |
| T 2,2-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T cis-1,2-Dichloroethene | 0.000 | | 0 | N.D. | | |
| T Methyl ethyl ketone | 0.000 | | 0 | N.D. | | |
| T Bromochloromethane | 0.000 | | 0 | N.D. | | |
| T Chloroform | 5.653 | 83.0 | 71551 | 52.2176 | ng | 98 |

Quantitation Results Report (QT Reviewed)





| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|-----------------------------|-------|-------|-------|--------|-------|----------|
| T 1,1,1-Trichloroethane | 0.000 | | 0 | N.D. | | |
| T Carbon tetrachloride | 6.029 | 117.0 | 1272 | 1.0055 | ng | m 96 |
| T 1,1-Dichloropropene | 0.000 | | 0 | N.D. | | |
| T Benzene | 6.286 | 78.0 | 1833 | 0.6395 | ng | m 90 |
| T 1,2-Dichloroethane | 6.317 | 62.0 | 0 | | ng | md 1 |
| T Trichloroethene | 0.000 | | 0 | N.D. | | |
| T 1,2-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T Dibromomethane | 0.000 | | 0 | N.D. | | |
| T Bromodichloromethane | 0.000 | | 0 | N.D. | | |
| T cis-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | |
| T Toluene | 8.383 | 92.0 | 260 | 0.1414 | ng | m 95 |
| T trans-1,3-Dichloropropene | 0.000 | | 0 | N.D. | | |
| T 1,1,2-Trichloroethane | 0.000 | | 0 | N.D. | | |
| T Tetrachloroethene | 0.000 | | 0 | N.D. | | |
| T 1,3-Dichloropropane | 0.000 | | 0 | N.D. | | |
| T Chlorodibromomethane | 0.000 | | 0 | N.D. | | |
| T 1,2-Dibromoethane | 0.000 | | 0 | N.D. | | |
| T Chlorobenzene | 0.000 | | 0 | N.D. | | |
| T 1,1,1,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | |
| T Ethylbenzene | 0.000 | | 0 | N.D. | | |
| T m+p-Xylenes | 0.000 | | 0 | N.D. | | |
| T o-Xylene | 0.000 | | 0 | N.D. | | |
| T Styrene | 0.000 | | 0 | N.D. | | |
| T Bromoform | 0.000 | | 0 | N.D. | | |
| T Bromobenzene | 0.000 | | 0 | N.D. | | |
| T 1,1,2,2-Tetrachloroethane | 0.000 | | 0 | N.D. | | |
| T 1,2,3-Trichloropropane | 0.000 | | 0 | N.D. | | |
| T 2-Chlorotoluene | 0.000 | | 0 | N.D. | | |
| T 4-Chlorotoluene | 0.000 | | 0 | N.D. | | |
| T 1,3-Dichlorobenzene | 0.000 | | 0 | N.D. | | |
| T 1,4-Dichlorobenzene | 0.000 | | 0 | N.D. | | |
| T 1,2-Dichlorobenzene | 0.000 | | 0 | N.D. | | |

(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)

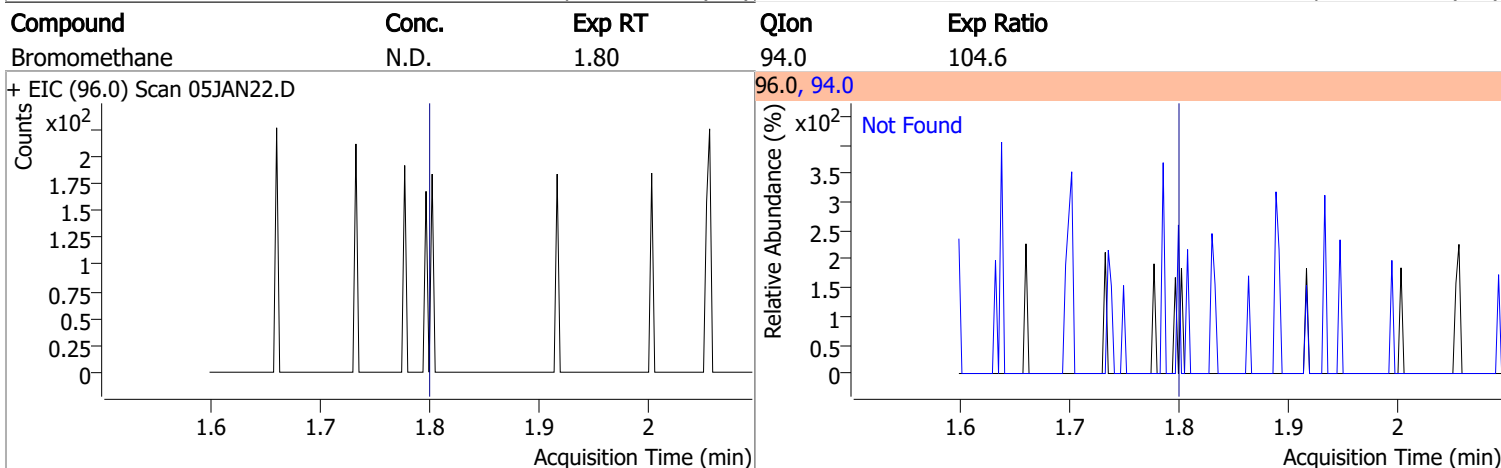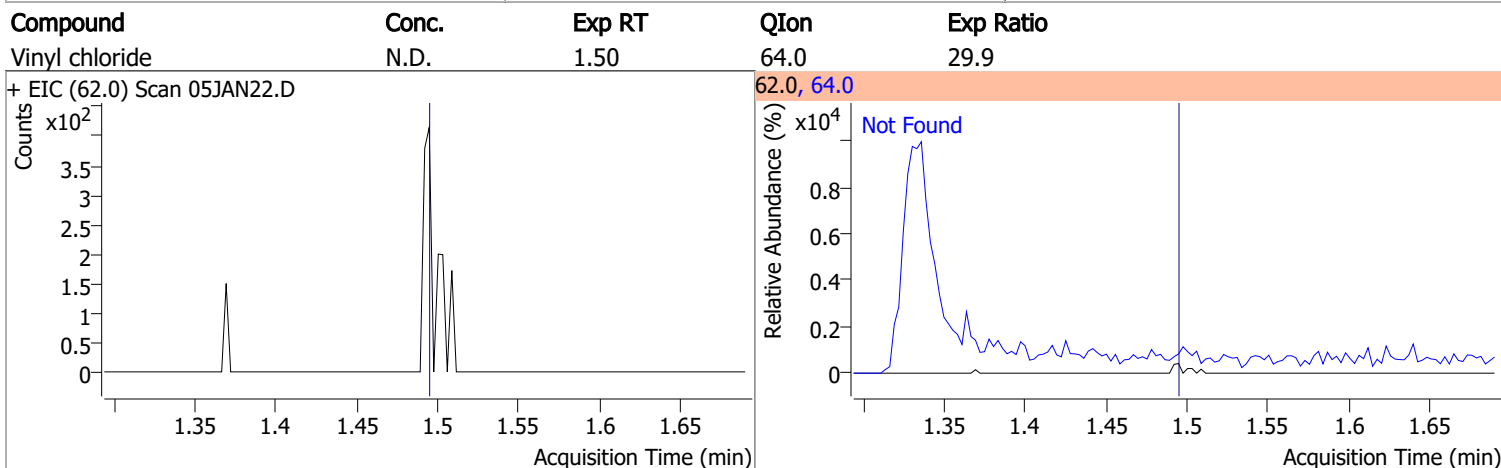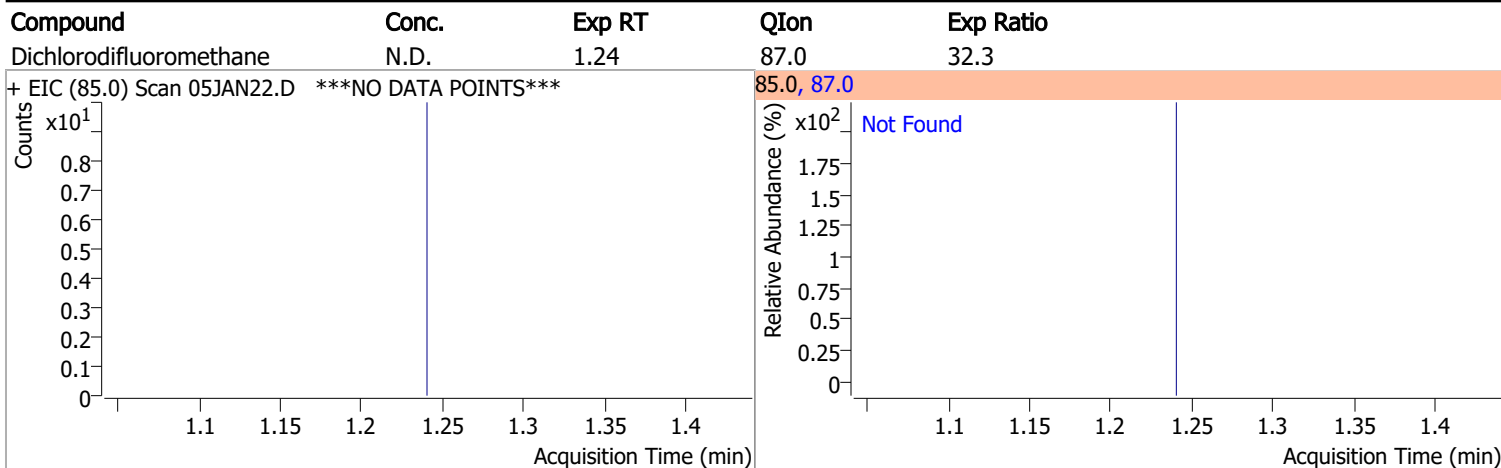


Quantitation Results Report (QT Reviewed)

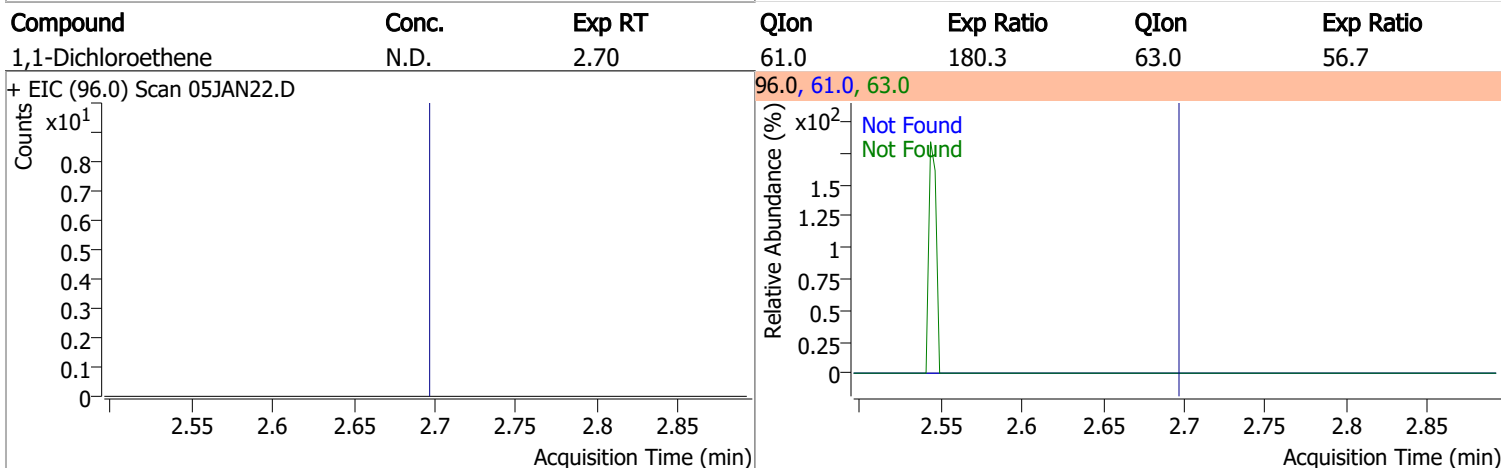


Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,2-Dichloroethene | N.D. | 3.72 | 61.0 | 153.9 | 98.0 | 65.7 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------------------|-------|--------|------|-----------|
| Methyl tert-butyl ether (MTBE) | N.D. | 3.75 | 57.0 | 24.6 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethane | N.D. | 4.38 | 65.0 | 32.1 | 83.0 | 13.7 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|------|-----------|
| 2,2-Dichloropropane | N.D. | 5.20 | 41.0 | 66.5 | 97.0 | 23.2 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|------------------------|-------|--------|------|-----------|------|-----------|
| cis-1,2-Dichloroethene | N.D. | 5.22 | 61.0 | 167.2 | 98.0 | 67.3 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| Methyl ethyl ketone | N.D. | 5.28 | 72.0 | 21.3 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|
| Bromochloromethane | N.D. | 5.52 | 49.0 | 182.9 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|---------|------|----------|-------|------|--------|-------|-------|
| Chloroform | 52.2176 | 5.65 | 0.00 | 71551 | 85.0 | 64.5 | 36.0 | 96.0 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------------|-------|--------|------|-----------|------|-----------|
| 1,1,1-Trichloroethane | N.D. | 5.83 | 99.0 | 64.7 | 61.0 | 48.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Dibromofluoromethane | 282.7463 | 5.85 | 0.00 | 191734 | 191.5 | 21.5 | 0.0 | 53.1 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|--------|------|----------|----------|-------|--------|-------|-------|
| Carbon tetrachloride | 1.0055 | 6.03 | 0.01 | 1272 (m) | 119.0 | 95.7 | 67.2 | 127.2 |
| | | | | | 121.0 | 22.6 | 0.1 | 60.1 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|-------|-----------|------|-----------|
| 1,1-Dichloropropene | N.D. | 6.04 | 110.0 | 35.9 | 77.0 | 30.1 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 287.7642 | 6.23 | 0.00 | 84285 | 65.0 | 197.6 | 166.5 | 226.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|--------|------|----------|----------|------|--------|-------|-------|
| Benzene | 0.6395 | 6.29 | 0.01 | 1833 (m) | 77.0 | 18.7 | 0.0 | 53.5 |











| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|-------|----|----------|-------|--------------|------------|------------|--------------|
| 1,2-Dichloroethane | 0 | 0 | 0 | 0 | 64.0 98.0 | 0.0 0.0 | 0.0 0.0 | 59.9 37.6 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------|-------|--------|-------|-----------|------|-----------|
| Trichloroethene | N.D. | 7.03 | 130.0 | 101.5 | 97.0 | 64.1 |




Quantitation Results Report (QT Reviewed)

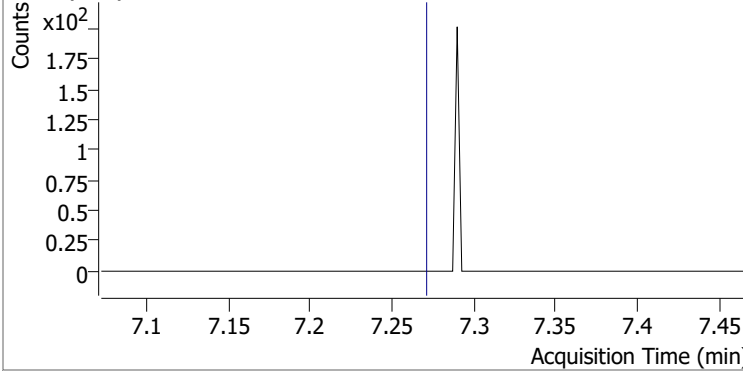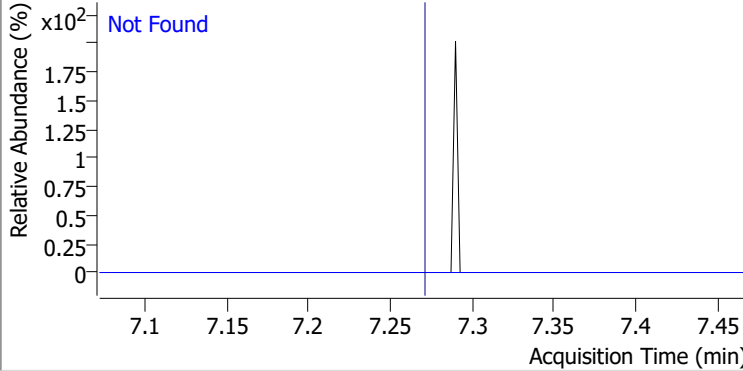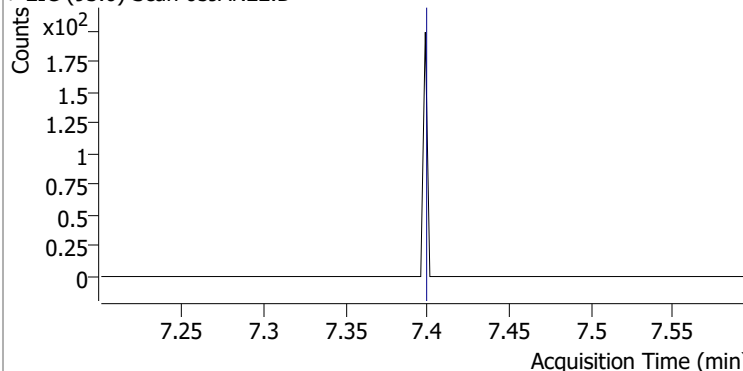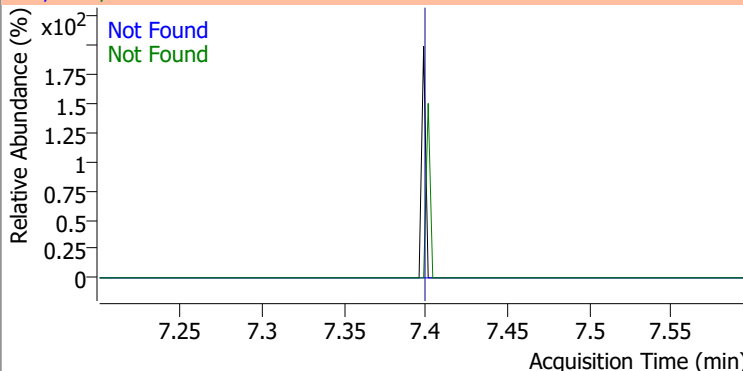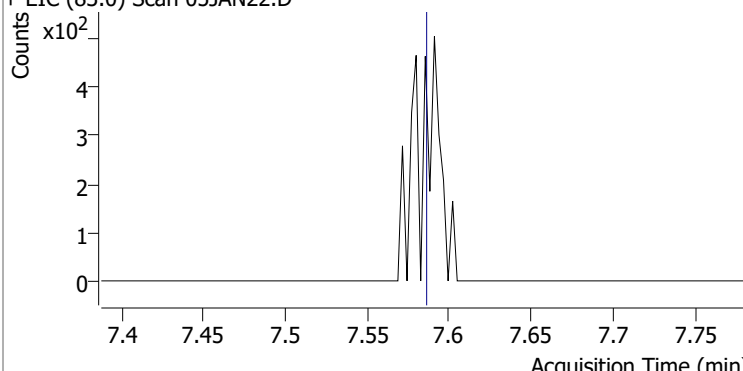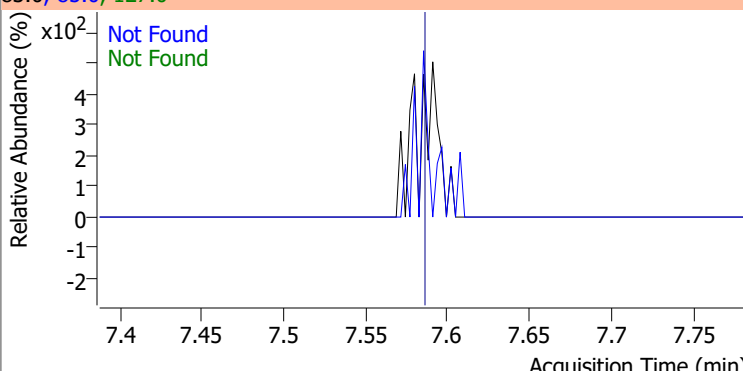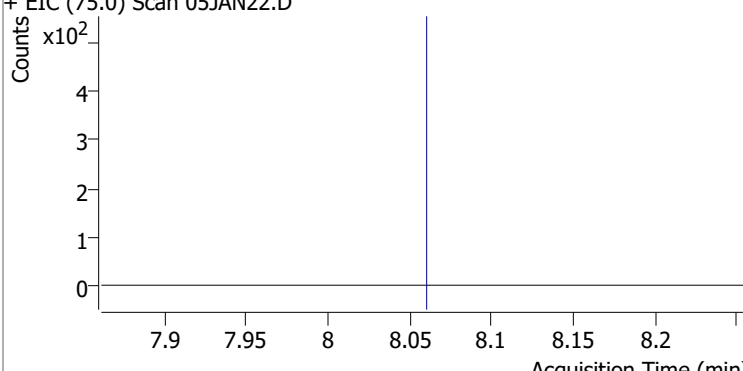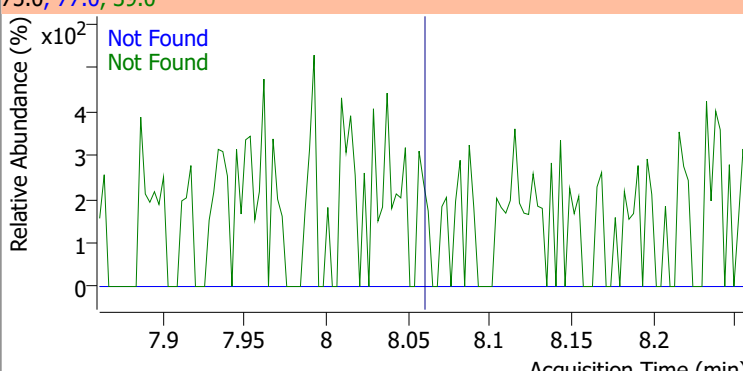
| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--|-------|--------|--|-----------|-------|-----------|
| 1,2-Dichloropropane | N.D. | 7.27 | 76.0 | 38.2 | | |
| + EIC (63.0) Scan 05JAN22.D | | | 63.0, 76.0 | | | |
|  | | |  | | | |
| Dibromomethane | N.D. | 7.40 | 173.5 | 113.7 | 95.0 | 82.2 |
| + EIC (93.0) Scan 05JAN22.D | | | 93.0, 95.0, 173.5 | | | |
|  | | |  | | | |
| Bromodichloromethane | N.D. | 7.59 | 85.0 | 64.5 | 127.0 | 9.6 |
| + EIC (83.0) Scan 05JAN22.D | | | 83.0, 85.0, 127.0 | | | |
|  | | |  | | | |
| cis-1,3-Dichloropropene | N.D. | 8.06 | 39.0 | 53.3 | 77.0 | 31.0 |
| + EIC (75.0) Scan 05JAN22.D | | | 75.0, 77.0, 39.0 | | | |
|  | | |  | | | |

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 264.6434 | 8.32 | 0.00 | 719407 | 100.0 | 63.9 | 34.4 | 94.4 |
| | | | | | 99.0 | 9.6 | 0.0 | 39.6 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|--------|------|----------|---------|------|--------|-------|-------|
| Toluene | 0.1414 | 8.38 | -0.01 | 260 (m) | 91.0 | 168.8 | 145.8 | 205.8 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,3-Dichloropropene | N.D. | 8.64 | 39.0 | 53.4 | 77.0 | 32.4 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------------|-------|--------|------|-----------|------|-----------|
| 1,1,2-Trichloroethane | N.D. | 8.82 | 97.0 | 114.6 | 85.0 | 67.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-------------------|-------|--------|-------|-----------|-------|-----------|
| Tetrachloroethene | N.D. | 8.94 | 165.8 | 128.6 | 129.0 | 91.5 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| 1,3-Dichloropropane | N.D. | 8.98 | 78.0 | 32.9 |



| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------------------|-------|--------|-------|-----------|
| Chlorodibromomethane | N.D. | 9.21 | 127.0 | 78.0 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|-------------------|-------|--------|-------|-----------|
| 1,2-Dibromoethane | N.D. | 9.31 | 109.0 | 94.5 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------|-------|--------|-------|-----------|
| Chlorobenzene | N.D. | 9.80 | 114.0 | 32.1 |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------------|-------|--------|-------|-----------|
| 1,1,1,2-Tetrachloroethane | N.D. | 9.89 | 133.0 | 98.6 |







| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|--------------|-------|--------|-------|-----------|
| Ethylbenzene | N.D. | 9.92 | 106.0 | 31.1 |











| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|-------------|-------|--------|------|-----------|
| m+p-Xylenes | N.D. | 10.04 | 91.0 | 201.4 |











Quantitation Results Report (QT Reviewed)



Quantitation Results Report (QT Reviewed)

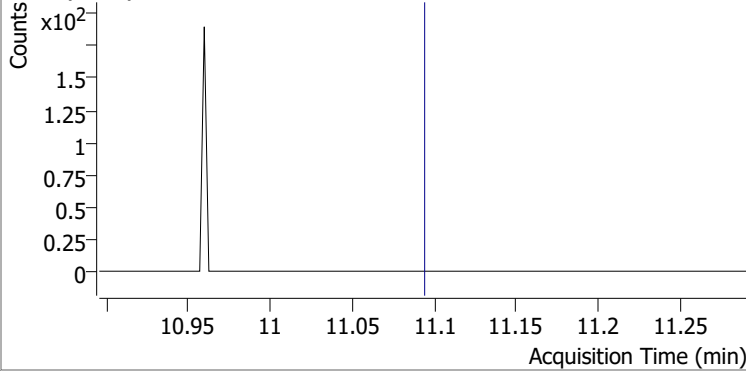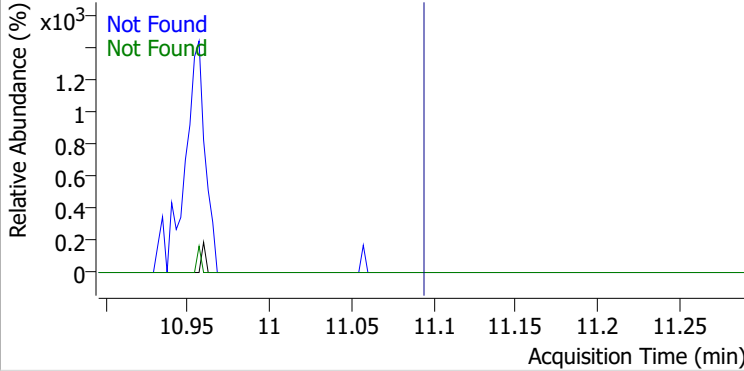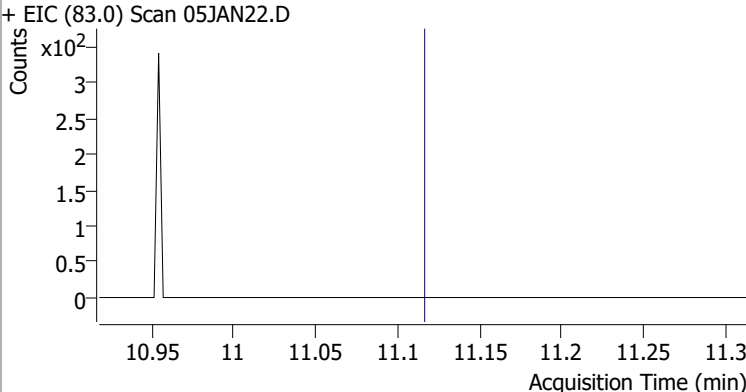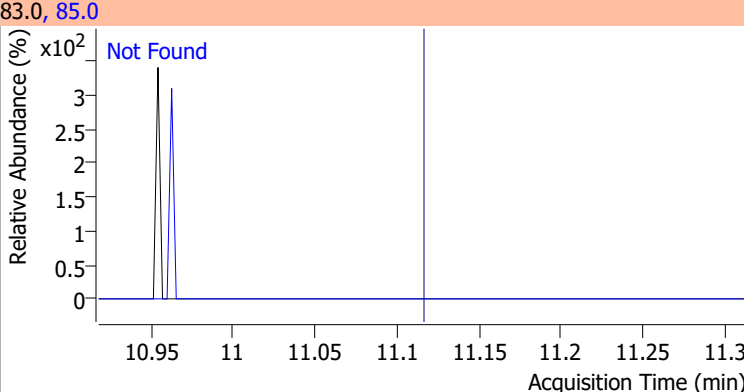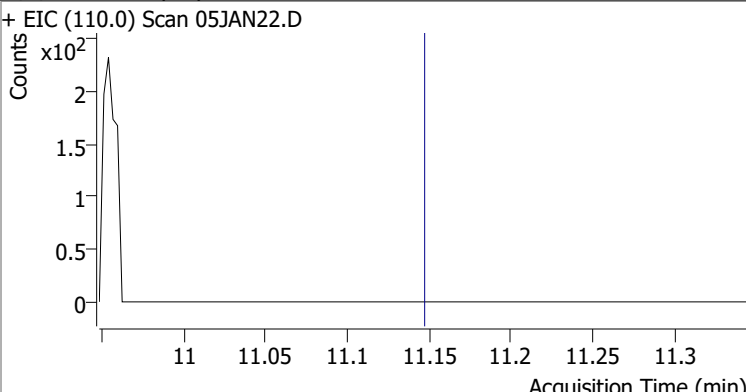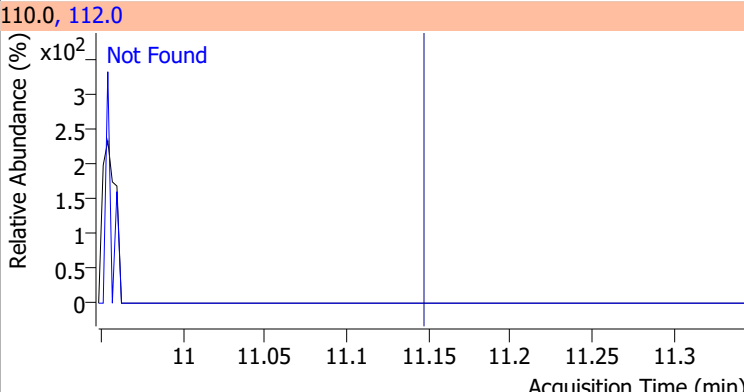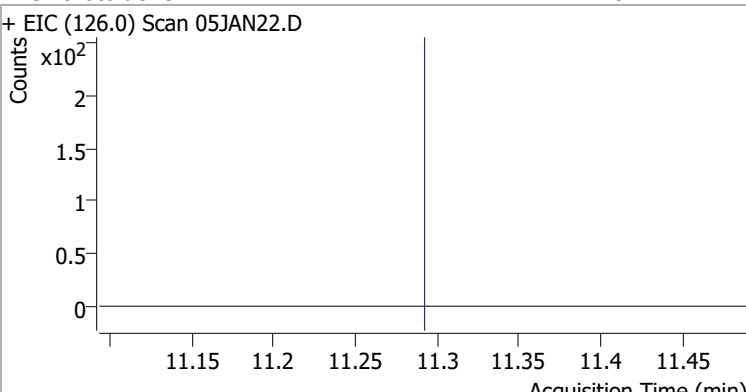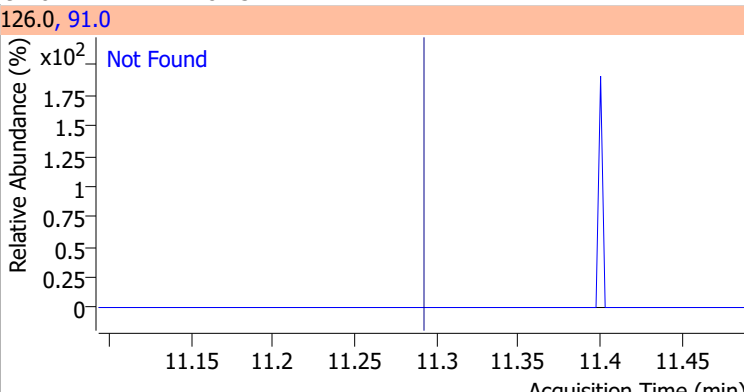
| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--|-------|--------|--|-----------|-------|-----------|
| Bromobenzene | N.D. | 11.09 | 77.0 | 145.7 | 158.0 | 96.5 |
| + EIC (156.0) Scan 05JAN22.D | | | 156.0, 77.0, 158.0 | | | |
|  | | |  | | | |
| 1,1,2,2-Tetrachloroethane | N.D. | 11.12 | 85.0 | 66.2 | | |
| + EIC (83.0) Scan 05JAN22.D | | | 83.0, 85.0 | | | |
|  | | |  | | | |
| 1,2,3-Trichloropropane | N.D. | 11.15 | 112.0 | 63.5 | | |
| + EIC (110.0) Scan 05JAN22.D | | | 110.0, 112.0 | | | |
|  | | |  | | | |
| 2-Chlorotoluene | N.D. | 11.29 | 91.0 | 282.3 | | |
| + EIC (126.0) Scan 05JAN22.D | | | 126.0, 91.0 | | | |
|  | | |  | | | |

Quantitation Results Report (QT Reviewed)
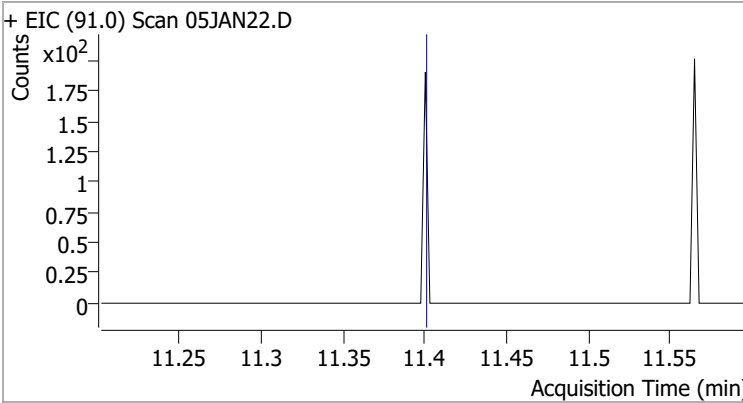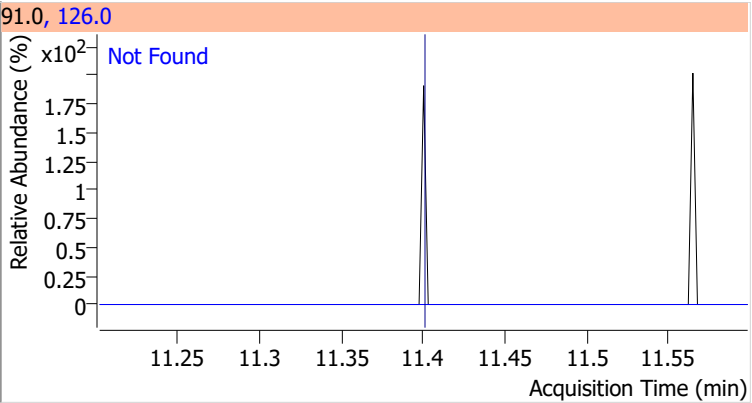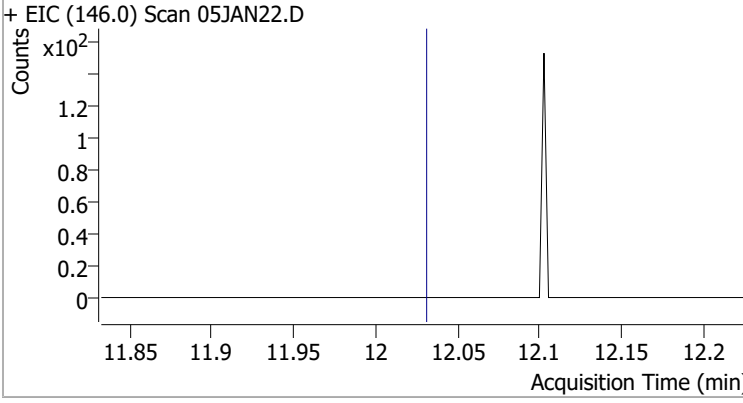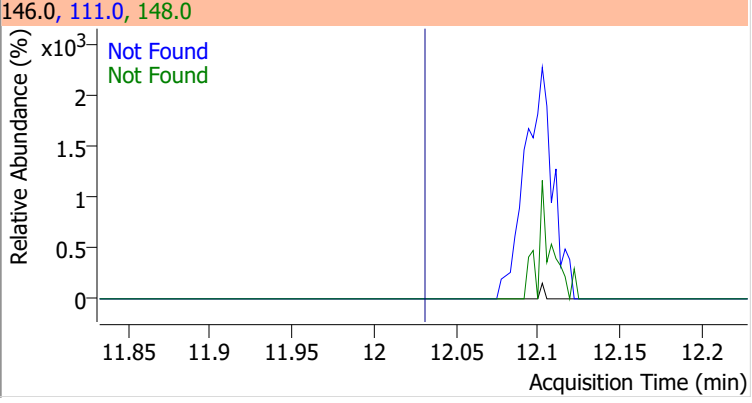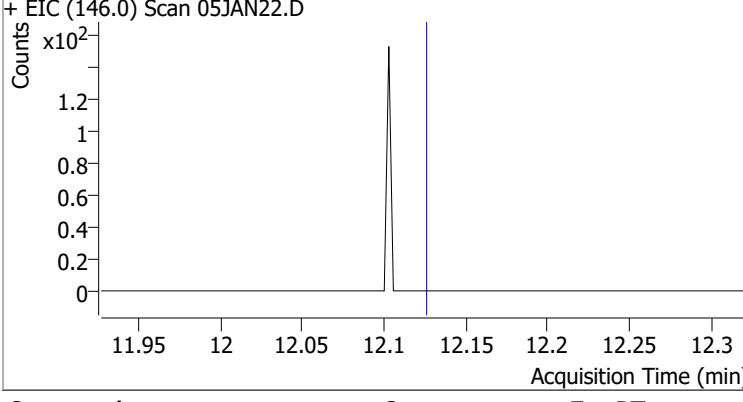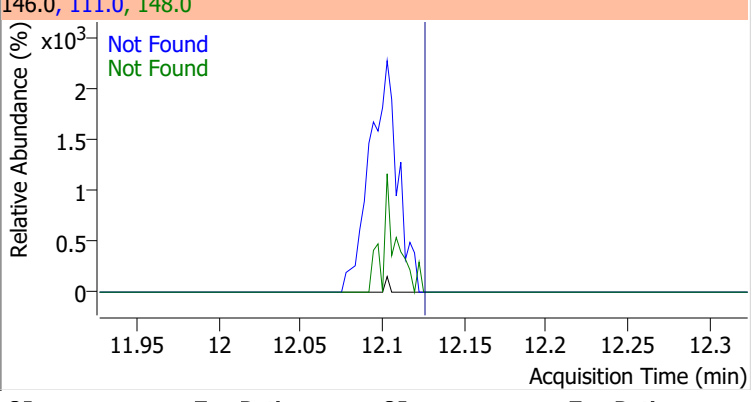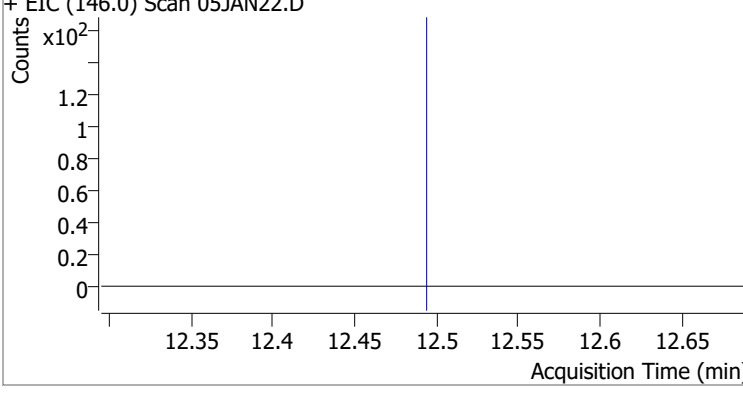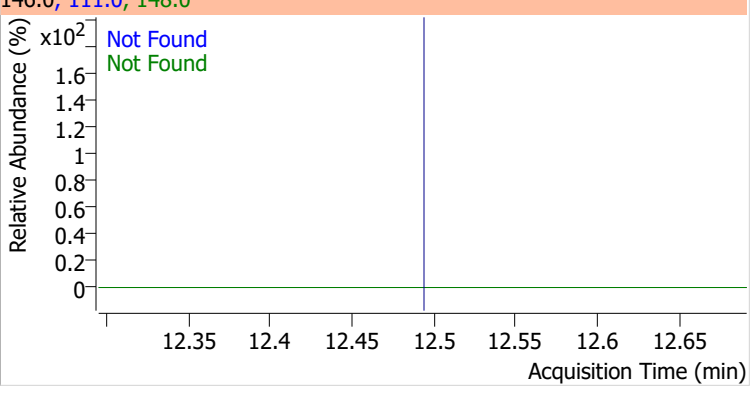
| Compound | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--|-------|--------|--|-----------|-------|-----------|
| 4-Chlorotoluene | N.D. | 11.40 | 126.0 | 31.7 | | |
| + EIC (91.0) Scan 05JAN22.D | | | 91.0, 126.0 | | | |
|  | | |  | | | |
| 1,3-Dichlorobenzene | N.D. | 12.03 | 148.0 | 63.6 | 111.0 | 39.8 |
| + EIC (146.0) Scan 05JAN22.D | | | 146.0, 111.0, 148.0 | | | |
|  | | |  | | | |
| 1,4-Dichlorobenzene | N.D. | 12.13 | 148.0 | 63.1 | 111.0 | 39.1 |
| + EIC (146.0) Scan 05JAN22.D | | | 146.0, 111.0, 148.0 | | | |
|  | | |  | | | |
| 1,2-Dichlorobenzene | N.D. | 12.49 | 148.0 | 63.9 | 111.0 | 41.0 |
| + EIC (146.0) Scan 05JAN22.D | | | 146.0, 111.0, 148.0 | | | |
|  | | |  | | | |

Quantitation Results Report (QT Reviewed)

| | | | |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File | 05JAN24.D | Operator | MSC |
| Acq. Method | 5975CACQF.M | Acq. Date-Time | 1/5/2022 8:33:23 PM |
| Sample Name | B22010002-001FMS | Instrument | VOA5975C |
| Vial | 24 | Multiplier | 1.00 |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m | Comment | |
| Tune File | BFB_Atune3.u | Tune Date | 10/11/2021 4:02:00 PM |
| Batch Name | VG010522_8260B.batch.bin | Last Calib Update | 2/28/2022 2:48:47 PM |
| Ref Library | \\MASSHUNTER\Org\Library\NIST129K.I | | |



| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|--------------------|-------|----------|
| Internal Standards | | | | | | |
| M Fluorobenzene | 6.620 | 96.0 | 756264 | 250.0000 | ng | -0.003 |
| M Chlorobenzene-d5 | 9.772 | 82.0 | 287819 | 250.0000 | ng | 0.000 |
| M 1,4-Dichlorobenzene-d4 | 12.100 | 152.0 | 241673 | 250.0000 | ng | 0.000 |
| System Monitoring Compounds | | | | | | |
| S Dibromofluoromethane | 5.845 | 113.0 | 195441 | 274.3119 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 80.0 - 119.0% | | | Recovery = 109.72% | | |
| S 1,2-Dichloroethane-d4 | 6.233 | 67.0 | 86697 | 281.7226 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 81.0 - 118.0% | | | Recovery = 112.69% | | |
| S Toluene-d8 | 8.319 | 98.0 | 774338 | 279.1845 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 89.0 - 112.0% | | | Recovery = 111.67% | | |
| S p-Bromofluorobenzene | 10.954 | 95.0 | 232802 | 262.9425 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 85.0 - 114.0% | | | Recovery = 105.18% | | |
| Target Compounds | | | | | | |
| T Dichlorodifluoromethane | 1.241 | 85.0 | 109042 | 110.0287 | ng | 99 |
| T Chloromethane | 1.406 | 50.0 | 127386 | 105.9017 | ng | 96 |
| T Vinyl chloride | 1.495 | 62.0 | 125903 | 116.3238 | ng | 96 |
| T Bromomethane | 1.796 | 96.0 | 50718 | 104.7949 | ng | 97 |
| T Chloroethane | 1.894 | 64.0 | 56380 | 105.2206 | ng | 99 |
| T Trichlorofluoromethane | 2.145 | 101.0 | 161834 | 120.4631 | ng | 98 |
| T 1,1-Dichloroethene | 2.702 | 96.0 | 99653 | 130.8181 | ng | 97 |
| T Methylene chloride | 3.333 | 49.0 | 135258 | 120.4467 | ng | 98 |
| T trans-1,2-Dichloroethene | 3.717 | 96.0 | 100073 | 128.7656 | ng | 99 |
| T Methyl tert-butyl ether (MTBE) | 3.756 | 73.0 | 136404 | 135.7867 | ng | 99 |
| T 1,1-Dichloroethane | 4.376 | 63.0 | 190421 | 131.6317 | ng | 99 |
| T 2,2-Dichloropropane | 5.190 | 77.0 | 135112 | 124.6457 | ng | 98 |
| T cis-1,2-Dichloroethene | 5.209 | 96.0 | 102488 | 130.0704 | ng | 95 |
| T Methyl ethyl ketone | 5.282 | 43.0 | 130330 | 1221.1260 | ng | 100 |
| T Bromochloromethane | 5.516 | 128.0 | 40412 | 123.8026 | ng | 98 |
| T Chloroform | 5.650 | 83.0 | 177003 | 122.9455 | ng | 98 |


Quantitation Results Report (QT Reviewed)

| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|-----------------------------|--------|-------|--------|----------|-------|----------|
| T 1,1,1-Trichloroethane | 5.828 | 97.0 | 171098 | 126.8131 | ng | 99 |
| T Carbon tetrachloride | 6.026 | 117.0 | 165149 | 124.2342 | ng | 100 |
| T 1,1-Dichloropropene | 6.040 | 75.0 | 136382 | 118.8843 | ng | 99 |
| T Benzene | 6.280 | 78.0 | 388978 | 129.1809 | ng | 99 |
| T 1,2-Dichloroethane | 6.319 | 62.0 | 100627 | 123.5320 | ng | 99 |
| T Trichloroethene | 7.025 | 95.0 | 110300 | 127.0700 | ng | 100 |
| T 1,2-Dichloropropane | 7.270 | 63.0 | 94289 | 123.4882 | ng | 97 |
| T Dibromomethane | 7.398 | 93.0 | 41507 | 128.6376 | ng | 97 |
| T Bromodichloromethane | 7.585 | 83.0 | 116127 | 130.4078 | ng | 100 |
| T cis-1,3-Dichloropropene | 8.059 | 75.0 | 115531 | 114.7487 | ng | 98 |
| T Toluene | 8.386 | 92.0 | 244059 | 130.2658 | ng | 99 |
| T trans-1,3-Dichloropropene | 8.639 | 75.0 | 91823 | 128.1244 | ng | 97 |
| T 1,1,2-Trichloroethane | 8.815 | 83.0 | 46926 | 125.7078 | ng | 97 |
| T Tetrachloroethene | 8.935 | 163.8 | 95413 | 124.8305 | ng | 100 |
| T 1,3-Dichloropropane | 8.977 | 76.0 | 89907 | 122.4461 | ng | 100 |
| T Chlorodibromomethane | 9.205 | 129.0 | 76710 | 131.4839 | ng | 97 |
| T 1,2-Dibromoethane | 9.309 | 107.0 | 50897 | 124.6965 | ng | 99 |
| T Chlorobenzene | 9.802 | 112.0 | 258411 | 125.9819 | ng | 99 |
| T 1,1,1,2-Tetrachloroethane | 9.891 | 131.0 | 89119 | 124.2913 | ng | 99 |
| T Ethylbenzene | 9.919 | 91.0 | 451644 | 126.9581 | ng | 99 |
| T m+p-Xylenes | 10.039 | 106.0 | 356274 | 257.7097 | ng | 99 |
| T o-Xylene | 10.430 | 106.0 | 159934 | 129.9530 | ng | 99 |
| T Styrene | 10.446 | 104.0 | 264262 | 133.3667 | ng | 99 |
| T Bromoform | 10.625 | 172.5 | 43697 | 141.2955 | ng | 99 |
| T Bromobenzene | 11.096 | 156.0 | 102340 | 130.8500 | ng | 99 |
| T 1,1,2,2-Tetrachloroethane | 11.116 | 83.0 | 58545 | 130.0529 | ng | 95 |
| T 1,2,3-Trichloropropane | 11.146 | 110.0 | 14953 | 124.1417 | ng | 99 |
| T 2-Chlorotoluene | 11.291 | 126.0 | 102259 | 131.4038 | ng | 99 |
| T 4-Chlorotoluene | 11.400 | 91.0 | 334790 | 131.9477 | ng | 100 |
| T 1,3-Dichlorobenzene | 12.033 | 146.0 | 183212 | 128.4415 | ng | 99 |
| T 1,4-Dichlorobenzene | 12.122 | 146.0 | 185434 | 127.4942 | ng | 99 |
| T 1,2-Dichlorobenzene | 12.493 | 146.0 | 153320 | 127.1837 | ng | 99 |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------------|----------|------|----------|--------|------|--------|-------|-------|
| Dichlorodifluoromethane | 110.0287 | 1.24 | 0.00 | 109042 | 87.0 | 31.5 | 2.3 | 62.3 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------|----------|------|----------|--------|------|--------|-------|-------|
| Chloromethane | 105.9017 | 1.41 | 0.00 | 127386 | 52.0 | 34.3 | 2.1 | 62.1 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------|----------|------|----------|--------|------|--------|-------|-------|
| Vinyl chloride | 116.3238 | 1.49 | 0.00 | 125903 | 64.0 | 32.1 | 0.0 | 59.9 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|----------|------|----------|-------|------|--------|-------|-------|
| Bromomethane | 104.7949 | 1.80 | 0.00 | 50718 | 94.0 | 107.4 | 74.6 | 134.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|----------|------|----------|-------|------|--------|-------|-------|
| Chloroethane | 105.2206 | 1.89 | 0.00 | 56380 | 66.0 | 30.4 | 0.1 | 60.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Trichlorofluoromethane | 120.4631 | 2.14 | 0.00 | 161834 | 103.0 | 66.0 | 34.2 | 94.2 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,1-Dichloroethene | 130.8181 | 2.70 | 0.01 | 99653 | 61.0 | 176.7 | 150.3 | 210.3 |
| | | | | | 63.0 | 54.1 | 26.7 | 86.7 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| Methylene chloride | 120.4467 | 3.33 | 0.00 | 135258 | 84.0 | 66.6 | 36.9 | 96.9 |
| | | | | | 86.0 | 42.1 | 14.3 | 74.3 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------------|----------|------|----------|--------|------|--------|-------|-------|
| trans-1,2-Dichloroethene | 128.7656 | 3.72 | 0.00 | 100073 | 61.0 | 156.3 | 123.9 | 183.9 |
| | | | | | 98.0 | 65.3 | 35.7 | 95.7 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------------------|----------|------|----------|--------|------|--------|-------|-------|
| Methyl tert-butyl ether (MTBE) | 135.7867 | 3.76 | 0.00 | 136404 | 57.0 | 24.3 | 0.0 | 54.6 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1-Dichloroethane | 131.6317 | 4.38 | 0.00 | 190421 | 65.0 | 31.5 | 2.1 | 62.1 |
| | | | | | 83.0 | 13.3 | 0.0 | 43.7 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 2,2-Dichloropropane | 124.6457 | 5.19 | -0.01 | 135112 | 41.0 | 68.1 | 36.5 | 96.5 |
| | | | | | 97.0 | 22.8 | 0.0 | 53.2 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,2-Dichloroethene | 130.0704 | 5.21 | -0.01 | 102488 | 61.0 | 160.6 | 137.2 | 197.2 |
| | | | | | 98.0 | 62.7 | 37.3 | 97.3 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|-----------|------|----------|--------|------|--------|-------|-------|
| Methyl ethyl ketone | 1221.1260 | 5.28 | 0.00 | 130330 | 72.0 | 21.2 | 0.0 | 51.3 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|-------|------|--------|-------|-------|
| Bromochloromethane | 123.8026 | 5.52 | 0.00 | 40412 | 49.0 | 185.6 | 152.9 | 212.9 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|------|--------|-------|-------|
| Chloroform | 122.9455 | 5.65 | 0.00 | 177003 | 85.0 | 64.4 | 36.0 | 96.0 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1,1-Trichloroethane | 126.8131 | 5.83 | -0.01 | 171098 | 99.0 | 63.4 | 34.7 | 94.7 |
| | | | | | 61.0 | 48.4 | 18.1 | 78.1 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Dibromofluoromethane | 274.3119 | 5.85 | 0.00 | 195441 | 191.5 | 22.0 | 0.0 | 53.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Carbon tetrachloride | 124.2342 | 6.03 | 0.00 | 165149 | 119.0 | 97.5 | 67.2 | 127.2 |
| | | | | | 121.0 | 30.2 | 0.1 | 60.1 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|-------|--------|-------|-------|
| 1,1-Dichloropropene | 118.8843 | 6.04 | 0.00 | 136382 | 110.0 | 35.1 | 5.9 | 65.9 |
| | | | | | 77.0 | 30.3 | 0.1 | 60.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 281.7226 | 6.23 | 0.00 | 86697 | 65.0 | 195.8 | 166.5 | 226.5 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|------|----------|--------|------|--------|-------|-------|
| Benzene | 129.1809 | 6.28 | 0.00 | 388978 | 77.0 | 23.1 | 0.0 | 53.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloroethane | 123.5320 | 6.32 | 0.00 | 100627 | 64.0 | 30.4 | 0.0 | 59.9 |
| | | | | | 98.0 | 8.3 | 0.0 | 37.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|----------|------|----------|--------|-------|--------|-------|-------|
| Trichloroethene | 127.0700 | 7.02 | -0.01 | 110300 | 130.0 | 101.4 | 71.5 | 131.5 |
| | | | | | 97.0 | 64.2 | 34.1 | 94.1 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloropropane | 123.4882 | 7.27 | 0.00 | 94289 | 76.0 | 40.3 | 8.2 | 68.2 |






| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------|----------|------|----------|-------|-------|--------|-------|-------|
| Dibromomethane | 128.6376 | 7.40 | 0.00 | 41507 | 173.5 | 108.1 | 83.7 | 143.7 |
| | | | | | 95.0 | 81.3 | 52.2 | 112.2 |






Quantitation Results Report (QT Reviewed)




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Bromodichloromethane | 130.4078 | 7.59 | 0.00 | 116127 | 85.0 | 64.5 | 34.5 | 94.5 |
| | | | | | 127.0 | 8.9 | 0.0 | 39.6 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,3-Dichloropropene | 114.7487 | 8.06 | 0.00 | 115531 | 39.0 | 54.2 | 23.3 | 83.3 |
| | | | | | 77.0 | 32.1 | 1.0 | 61.0 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 279.1845 | 8.32 | 0.00 | 774338 | 100.0 | 62.9 | 34.4 | 94.4 |
| | | | | | 99.0 | 9.5 | 0.0 | 39.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|------|----------|--------|------|--------|-------|-------|
| Toluene | 130.2658 | 8.39 | 0.00 | 244059 | 91.0 | 174.0 | 145.8 | 205.8 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|----------|------|----------|-------|------|--------|-------|-------|
| trans-1,3-Dichloropropene | 128.1244 | 8.64 | 0.00 | 91823 | 39.0 | 50.3 | 23.4 | 83.4 |
| | | | | | 77.0 | 31.8 | 2.4 | 62.4 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,1,2-Trichloroethane | 125.7078 | 8.82 | 0.00 | 46926 | 97.0 | 113.0 | 84.6 | 144.6 |
| | | | | | 85.0 | 62.9 | 37.6 | 97.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------|----------|------|----------|-------|-------|--------|-------|-------|
| Tetrachloroethene | 124.8305 | 8.93 | 0.00 | 95413 | 165.8 | 128.3 | 98.6 | 158.6 |
| | | | | | 129.0 | 91.8 | 61.5 | 121.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,3-Dichloropropane | 122.4461 | 8.98 | 0.00 | 89907 | 78.0 | 33.1 | 2.9 | 62.9 |















| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|-------|-------|--------|-------|-------|
| Chlorodibromomethane | 131.4839 | 9.21 | 0.00 | 76710 | 127.0 | 75.8 | 48.0 | 108.0 |







| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------|----------|------|----------|-------|-------|--------|-------|-------|
| 1,2-Dibromoethane | 124.6965 | 9.31 | 0.00 | 50897 | 109.0 | 95.9 | 64.5 | 124.5 |



Quantitation Results Report (QT Reviewed)

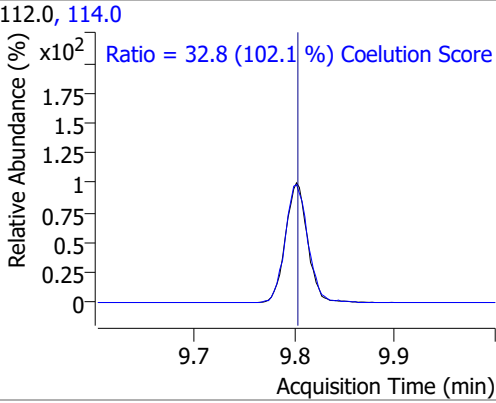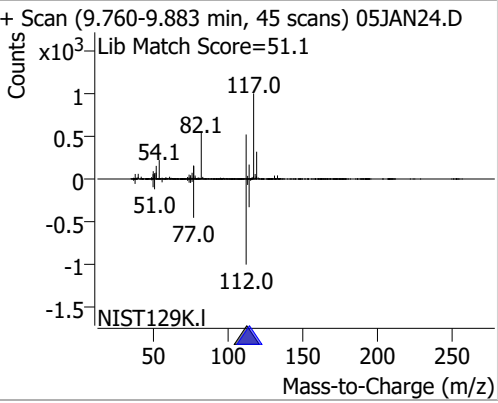
| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--|----------|-------|---|--------|-------|--|-------|-------|
| Chlorobenzene | 125.9819 | 9.80 | 0.00 | 258411 | 114.0 | 32.8 | 2.1 | 62.1 |
| + EIC (112.0) Scan 05JAN24.D  | | | 112.0, 114.0  | | | + Scan (9.760-9.883 min, 45 scans) 05JAN24.D Lib Match Score=51.1  | | |
| 1,1,1,2-Tetrachloroethane | 124.2913 | 9.89 | 0.00 | 89119 | 133.0 | 97.7 | 68.6 | 128.6 |
| + EIC (131.0) Scan 05JAN24.D  | | | 131.0, 133.0  | | | + Scan (9.852-9.956 min, 38 scans) 05JAN24.D Lib Match Score=60.1  | | |
| Ethylbenzene | 126.9581 | 9.92 | 0.00 | 451644 | 106.0 | 31.4 | 1.1 | 61.1 |
| + EIC (91.0) Scan 05JAN24.D  | | | 91.0, 106.0  | | | + Scan (9.875-9.995 min, 44 scans) 05JAN24.D Lib Match Score=62.1  | | |
| m+p-Xylenes | 257.7097 | 10.04 | 0.00 | 356274 | 91.0 | 203.0 | 171.4 | 231.4 |
| + EIC (106.0) Scan 05JAN24.D  | | | 106.0, 91.0  | | | + Scan (9.989-10.109 min, 43 scans) 05JAN24.D Lib Match Score=62.1  | | |

Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|----------|-------|----------|--------|-------|--------|-------|-------|
| Bromobenzene | 130.8500 | 11.10 | 0.00 | 102340 | 77.0 | 143.9 | 115.7 | 175.7 |
| | | | | | 158.0 | 96.5 | 66.5 | 126.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|----------|-------|----------|-------|------|--------|-------|-------|
| 1,1,2,2-Tetrachloroethane | 130.0529 | 11.12 | 0.00 | 58545 | 85.0 | 62.5 | 36.2 | 96.2 |












| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|----------|-------|----------|-------|-------|--------|-------|-------|
| 1,2,3-Trichloropropane | 124.1417 | 11.15 | 0.00 | 14953 | 112.0 | 62.9 | 33.5 | 93.5 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|----------|-------|----------|--------|------|--------|-------|-------|
| 2-Chlorotoluene | 131.4038 | 11.29 | 0.00 | 102259 | 91.0 | 280.2 | 252.3 | 312.3 |






Quantitation Results Report (QT Reviewed)
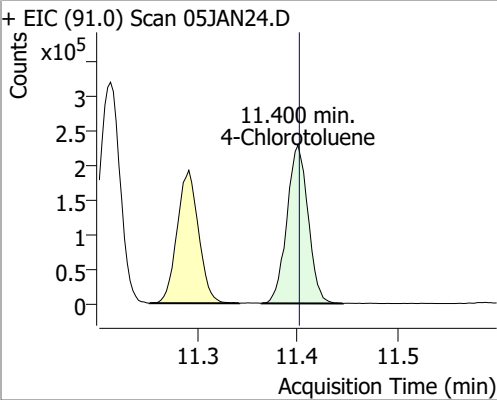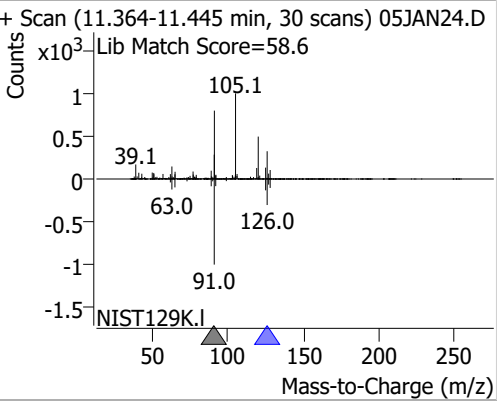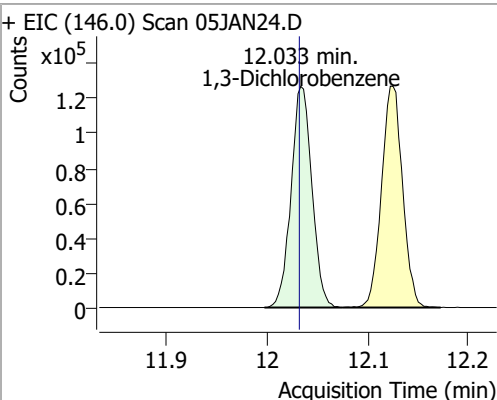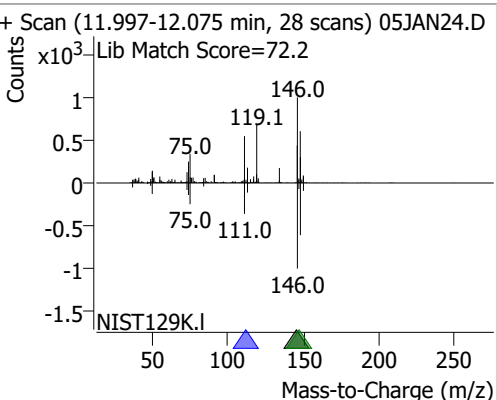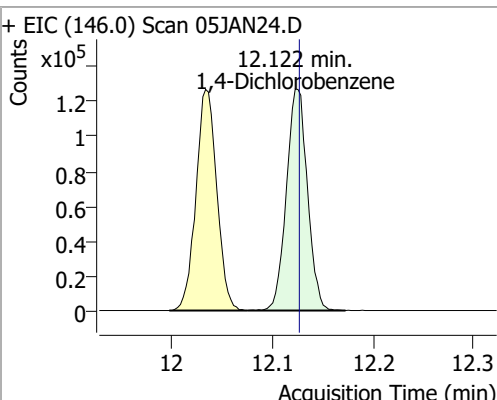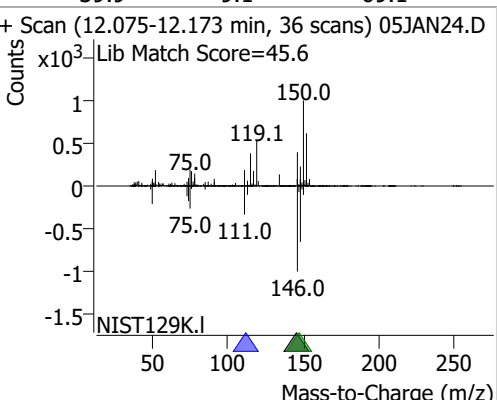
| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--|----------|-------|---|--------|-------|---|-------|-------|
| 4-Chlorotoluene | 131.9477 | 11.40 | 0.00 | 334790 | 126.0 | 31.9 | 1.7 | 61.7 |
| + EIC (91.0) Scan 05JAN24.D  | | | 91.0, 126.0  | | | + Scan (11.364-11.445 min, 30 scans) 05JAN24.D Lib Match Score=58.6  | | |
| 1,3-Dichlorobenzene | 128.4415 | 12.03 | 0.00 | 183212 | 148.0 | 63.4 | 33.6 | 93.6 |
| + EIC (146.0) Scan 05JAN24.D  | | | 146.0, 111.0, 148.0  | | | + Scan (11.997-12.075 min, 28 scans) 05JAN24.D Lib Match Score=72.2  | | |
| 1,4-Dichlorobenzene | 127.4942 | 12.12 | 0.00 | 185434 | 148.0 | 63.1 | 33.1 | 93.1 |
| + EIC (146.0) Scan 05JAN24.D  | | | 146.0, 111.0, 148.0  | | | + Scan (12.075-12.173 min, 36 scans) 05JAN24.D Lib Match Score=45.6  | | |


Quantitation Results Report (QT Reviewed)

| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,2-Dichlorobenzene | 127.1837 | 12.49 | 0.00 | 153320 | 148.0 | 62.5 | 33.9 | 93.9 |
| | | | | | 111.0 | 40.6 | 11.0 | 71.0 |



Quantitation Results Report (QT Reviewed)

| | | | |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File | 05JAN25.D | Operator | MSC |
| Acq. Method | 5975CACQF.M | Acq. Date-Time | 1/5/2022 9:00:38 PM |
| Sample Name | B22010002-001FMSD | Instrument | VOA5975C |
| Vial | 25 | Multiplier | 1.00 |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m | Comment | |
| Tune File | BFB_Atune3.u | Tune Date | 10/11/2021 4:02:00 PM |
| Batch Name | VG010522_8260B.batch.bin | Last Calib Update | 2/28/2022 2:48:47 PM |
| Ref Library | \\MASSHUNTER\Org\Library\NIST129K.I | | |



| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|--------------------|-------|----------|
| Internal Standards | | | | | | |
| M Fluorobenzene | 6.620 | 96.0 | 774748 | 250.0000 | ng | -0.003 |
| M Chlorobenzene-d5 | 9.774 | 82.0 | 299679 | 250.0000 | ng | 0.003 |
| M 1,4-Dichlorobenzene-d4 | 12.100 | 152.0 | 246742 | 250.0000 | ng | 0.000 |
| System Monitoring Compounds | | | | | | |
| S Dibromofluoromethane | 5.845 | 113.0 | 199345 | 273.1160 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 80.0 - 119.0% | | | Recovery = 109.25% | | |
| S 1,2-Dichloroethane-d4 | 6.233 | 67.0 | 89260 | 283.1311 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 81.0 - 118.0% | | | Recovery = 113.25% | | |
| S Toluene-d8 | 8.322 | 98.0 | 797612 | 276.1949 | ng | 0.003 |
| Spiked Amount: 250.000 | Range: 89.0 - 112.0% | | | Recovery = 110.48% | | |
| S p-Bromofluorobenzene | 10.951 | 95.0 | 243414 | 269.2804 | ng | -0.003 |
| Spiked Amount: 250.000 | Range: 85.0 - 114.0% | | | Recovery = 107.71% | | |
| Target Compounds | | | | | | |
| T Dichlorodifluoromethane | 1.241 | 85.0 | 118927 | 117.1401 | ng | 100 |
| T Chloromethane | 1.408 | 50.0 | 142908 | 115.9713 | ng | 99 |
| T Vinyl chloride | 1.495 | 62.0 | 140829 | 127.0099 | ng | 97 |
| T Bromomethane | 1.799 | 96.0 | 59143 | 119.2874 | ng | 98 |
| T Chloroethane | 1.894 | 64.0 | 62164 | 113.2473 | ng | 99 |
| T Trichlorofluoromethane | 2.145 | 101.0 | 167114 | 121.4256 | ng | 99 |
| T 1,1-Dichloroethene | 2.700 | 96.0 | 109427 | 140.2216 | ng | 99 |
| T Methylene chloride | 3.330 | 49.0 | 145652 | 126.6081 | ng | 99 |
| T trans-1,2-Dichloroethene | 3.717 | 96.0 | 111580 | 140.1465 | ng | 99 |
| T Methyl tert-butyl ether (MTBE) | 3.751 | 73.0 | 147515 | 143.3439 | ng | 99 |
| T 1,1-Dichloroethane | 4.376 | 63.0 | 211672 | 142.8308 | ng | 99 |
| T 2,2-Dichloropropane | 5.195 | 77.0 | 147122 | 132.4872 | ng | 98 |
| T cis-1,2-Dichloroethene | 5.215 | 96.0 | 111323 | 137.9124 | ng | 98 |
| T Methyl ethyl ketone | 5.279 | 43.0 | 144644 | 1322.9075 | ng | 98 |
| T Bromochloromethane | 5.519 | 128.0 | 44732 | 133.7676 | ng | 100 |
| T Chloroform | 5.647 | 83.0 | 189725 | 128.6381 | ng | 100 |


Quantitation Results Report (QT Reviewed)

| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|-----------------------------|--------|-------|--------|----------|-------|----------|
| T 1,1,1-Trichloroethane | 5.831 | 97.0 | 188353 | 136.2713 | ng | 100 |
| T Carbon tetrachloride | 6.026 | 117.0 | 180517 | 132.5551 | ng | 99 |
| T 1,1-Dichloropropene | 6.040 | 75.0 | 151786 | 129.1553 | ng | 98 |
| T Benzene | 6.277 | 78.0 | 420571 | 136.3407 | ng | 100 |
| T 1,2-Dichloroethane | 6.325 | 62.0 | 111944 | 134.1463 | ng | 98 |
| T Trichloroethene | 7.025 | 95.0 | 119213 | 131.9029 | ng | 98 |
| T 1,2-Dichloropropane | 7.273 | 63.0 | 105821 | 133.1065 | ng | 99 |
| T Dibromomethane | 7.398 | 93.0 | 44225 | 131.6369 | ng | 98 |
| T Bromodichloromethane | 7.583 | 83.0 | 128815 | 138.9313 | ng | 99 |
| T cis-1,3-Dichloropropene | 8.057 | 75.0 | 131596 | 125.5322 | ng | 99 |
| T Toluene | 8.388 | 92.0 | 265405 | 136.0530 | ng | 99 |
| T trans-1,3-Dichloropropene | 8.637 | 75.0 | 102973 | 137.9961 | ng | 96 |
| T 1,1,2-Trichloroethane | 8.815 | 83.0 | 50972 | 131.1425 | ng | 99 |
| T Tetrachloroethene | 8.935 | 163.8 | 104953 | 131.8777 | ng | 99 |
| T 1,3-Dichloropropane | 8.977 | 76.0 | 101137 | 132.2893 | ng | 99 |
| T Chlorodibromomethane | 9.203 | 129.0 | 86755 | 142.8165 | ng | 97 |
| T 1,2-Dibromoethane | 9.306 | 107.0 | 58242 | 137.0445 | ng | 99 |
| T Chlorobenzene | 9.799 | 112.0 | 287977 | 134.8398 | ng | 100 |
| T 1,1,1,2-Tetrachloroethane | 9.892 | 131.0 | 96722 | 129.5564 | ng | 98 |
| T Ethylbenzene | 9.917 | 91.0 | 495112 | 133.6690 | ng | 99 |
| T m+p-Xylenes | 10.039 | 106.0 | 388623 | 269.9841 | ng | 100 |
| T o-Xylene | 10.433 | 106.0 | 176516 | 137.7503 | ng | 98 |
| T Styrene | 10.449 | 104.0 | 283898 | 137.6062 | ng | 98 |
| T Bromoform | 10.628 | 172.5 | 50331 | 159.4033 | ng | 97 |
| T Bromobenzene | 11.093 | 156.0 | 108389 | 135.7371 | ng | 98 |
| T 1,1,2,2-Tetrachloroethane | 11.110 | 83.0 | 63810 | 138.8366 | ng | 99 |
| T 1,2,3-Trichloropropane | 11.149 | 110.0 | 17155 | 139.4971 | ng | 95 |
| T 2-Chlorotoluene | 11.291 | 126.0 | 111355 | 140.1526 | ng | 99 |
| T 4-Chlorotoluene | 11.397 | 91.0 | 364459 | 140.6899 | ng | 100 |
| T 1,3-Dichlorobenzene | 12.036 | 146.0 | 198469 | 136.2791 | ng | 99 |
| T 1,4-Dichlorobenzene | 12.122 | 146.0 | 199434 | 134.3028 | ng | 99 |
| T 1,2-Dichlorobenzene | 12.493 | 146.0 | 168422 | 136.8411 | ng | 98 |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------------|----------|------|----------|--------|------|--------|-------|-------|
| Dichlorodifluoromethane | 117.1401 | 1.24 | 0.00 | 118927 | 87.0 | 32.2 | 2.3 | 62.3 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------|----------|------|----------|--------|------|--------|-------|-------|
| Chloromethane | 115.9713 | 1.41 | 0.00 | 142908 | 52.0 | 32.5 | 2.1 | 62.1 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------|----------|------|----------|--------|------|--------|-------|-------|
| Vinyl chloride | 127.0099 | 1.49 | 0.00 | 140829 | 64.0 | 31.5 | 0.0 | 59.9 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|----------|------|----------|-------|------|--------|-------|-------|
| Bromomethane | 119.2874 | 1.80 | 0.00 | 59143 | 94.0 | 102.7 | 74.6 | 134.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|----------|------|----------|-------|------|--------|-------|-------|
| Chloroethane | 113.2473 | 1.89 | 0.00 | 62164 | 66.0 | 30.4 | 0.1 | 60.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Trichlorofluoromethane | 121.4256 | 2.14 | 0.00 | 167114 | 103.0 | 65.3 | 34.2 | 94.2 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1-Dichloroethene | 140.2216 | 2.70 | 0.00 | 109427 | 61.0 | 182.1 | 150.3 | 210.3 |
| | | | | | 63.0 | 58.0 | 26.7 | 86.7 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| Methylene chloride | 126.6081 | 3.33 | -0.01 | 145652 | 84.0 | 67.7 | 36.9 | 96.9 |
| | | | | | 86.0 | 43.2 | 14.3 | 74.3 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------------|----------|------|----------|--------|------|--------|-------|-------|
| trans-1,2-Dichloroethene | 140.1465 | 3.72 | 0.00 | 111580 | 61.0 | 153.9 | 123.9 | 183.9 |
| | | | | | 98.0 | 62.4 | 35.7 | 95.7 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------------------|----------|------|----------|--------|------|--------|-------|-------|
| Methyl tert-butyl ether (MTBE) | 143.3439 | 3.75 | 0.00 | 147515 | 57.0 | 25.2 | 0.0 | 54.6 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1-Dichloroethane | 142.8308 | 4.38 | 0.00 | 211672 | 65.0 | 31.9 | 2.1 | 62.1 |
| | | | | | 83.0 | 12.8 | 0.0 | 43.7 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 2,2-Dichloropropane | 132.4872 | 5.20 | 0.00 | 147122 | 41.0 | 69.0 | 36.5 | 96.5 |
| | | | | | 97.0 | 23.3 | 0.0 | 53.2 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,2-Dichloroethene | 137.9124 | 5.21 | 0.00 | 111323 | 61.0 | 163.7 | 137.2 | 197.2 |
| | | | | | 98.0 | 66.3 | 37.3 | 97.3 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|-----------|------|----------|--------|------|--------|-------|-------|
| Methyl ethyl ketone | 1322.9075 | 5.28 | 0.00 | 144644 | 72.0 | 22.1 | 0.0 | 51.3 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|-------|------|--------|-------|-------|
| Bromochloromethane | 133.7676 | 5.52 | 0.00 | 44732 | 49.0 | 183.4 | 152.9 | 212.9 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|------|--------|-------|-------|
| Chloroform | 128.6381 | 5.65 | -0.01 | 189725 | 85.0 | 66.3 | 36.0 | 96.0 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1,1-Trichloroethane | 136.2713 | 5.83 | 0.00 | 188353 | 99.0 | 64.6 | 34.7 | 94.7 |
| | | | | | 61.0 | 47.9 | 18.1 | 78.1 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Dibromofluoromethane | 273.1160 | 5.85 | 0.00 | 199345 | 191.5 | 21.8 | 0.0 | 53.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Carbon tetrachloride | 132.5551 | 6.03 | 0.00 | 180517 | 119.0 | 97.6 | 67.2 | 127.2 |
| | | | | | 121.0 | 31.6 | 0.1 | 60.1 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|-------|--------|-------|-------|
| 1,1-Dichloropropene | 129.1553 | 6.04 | 0.00 | 151786 | 110.0 | 37.4 | 5.9 | 65.9 |
| | | | | | 77.0 | 30.9 | 0.1 | 60.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 283.1311 | 6.23 | 0.00 | 89260 | 65.0 | 198.4 | 166.5 | 226.5 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|------|----------|--------|------|--------|-------|-------|
| Benzene | 136.3407 | 6.28 | 0.00 | 420571 | 77.0 | 23.3 | 0.0 | 53.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloroethane | 134.1463 | 6.32 | 0.00 | 111944 | 64.0 | 31.1 | 0.0 | 59.9 |
| | | | | | 98.0 | 8.2 | 0.0 | 37.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|----------|------|----------|--------|-------|--------|-------|-------|
| Trichloroethene | 131.9029 | 7.02 | -0.01 | 119213 | 130.0 | 103.5 | 71.5 | 131.5 |
| | | | | | 97.0 | 65.2 | 34.1 | 94.1 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloropropane | 133.1065 | 7.27 | 0.00 | 105821 | 76.0 | 39.0 | 8.2 | 68.2 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------|----------|------|----------|-------|-------|--------|-------|-------|
| Dibromomethane | 131.6369 | 7.40 | 0.00 | 44225 | 173.5 | 112.5 | 83.7 | 143.7 |
| | | | | | 95.0 | 85.7 | 52.2 | 112.2 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Bromodichloromethane | 138.9313 | 7.58 | 0.00 | 128815 | 85.0 | 63.5 | 34.5 | 94.5 |
| | | | | | 127.0 | 9.4 | 0.0 | 39.6 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,3-Dichloropropene | 125.5322 | 8.06 | 0.00 | 131596 | 39.0 | 53.4 | 23.3 | 83.3 |
| | | | | | 77.0 | 31.7 | 1.0 | 61.0 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 276.1949 | 8.32 | 0.00 | 797612 | 100.0 | 63.8 | 34.4 | 94.4 |
| | | | | | 99.0 | 9.4 | 0.0 | 39.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|------|----------|--------|------|--------|-------|-------|
| Toluene | 136.0530 | 8.39 | 0.00 | 265405 | 91.0 | 174.6 | 145.8 | 205.8 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|----------|------|----------|--------|------|--------|-------|-------|
| trans-1,3-Dichloropropene | 137.9961 | 8.64 | 0.00 | 102973 | 39.0 | 49.9 | 23.4 | 83.4 |
| | | | | | 77.0 | 31.5 | 2.4 | 62.4 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,1,2-Trichloroethane | 131.1425 | 8.82 | 0.00 | 50972 | 97.0 | 113.5 | 84.6 | 144.6 |
| | | | | | 85.0 | 66.0 | 37.6 | 97.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Tetrachloroethene | 131.8777 | 8.94 | 0.00 | 104953 | 165.8 | 128.4 | 98.6 | 158.6 |
| | | | | | 129.0 | 89.0 | 61.5 | 121.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,3-Dichloropropane | 132.2893 | 8.98 | 0.00 | 101137 | 78.0 | 32.4 | 2.9 | 62.9 |







| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|-------|-------|--------|-------|-------|
| Chlorodibromomethane | 142.8165 | 9.20 | 0.00 | 86755 | 127.0 | 75.5 | 48.0 | 108.0 |







| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------|----------|------|----------|-------|-------|--------|-------|-------|
| 1,2-Dibromoethane | 137.0445 | 9.31 | 0.00 | 58242 | 109.0 | 93.2 | 64.5 | 124.5 |



Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|----------|-------|----------|--------|-------|--------|-------|-------|
| Bromobenzene | 135.7371 | 11.09 | 0.00 | 108389 | 77.0 | 147.1 | 115.7 | 175.7 |
| | | | | | 158.0 | 99.8 | 66.5 | 126.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|----------|-------|----------|-------|------|--------|-------|-------|
| 1,1,2,2-Tetrachloroethane | 138.8366 | 11.11 | -0.01 | 63810 | 85.0 | 65.2 | 36.2 | 96.2 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|----------|-------|----------|-------|-------|--------|-------|-------|
| 1,2,3-Trichloropropane | 139.4971 | 11.15 | 0.00 | 17155 | 112.0 | 59.6 | 33.5 | 93.5 |






| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|----------|-------|----------|--------|------|--------|-------|-------|
| 2-Chlorotoluene | 140.1526 | 11.29 | 0.00 | 111355 | 91.0 | 284.3 | 252.3 | 312.3 |






Quantitation Results Report (QT Reviewed)




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 4-Chlorotoluene | 140.6899 | 11.40 | 0.00 | 364459 | 126.0 | 31.7 | 1.7 | 61.7 |



| | | | | | | | | |
|---------------------|----------|-------|------|--------|-------|------|------|------|
| 1,3-Dichlorobenzene | 136.2791 | 12.04 | 0.01 | 198469 | 148.0 | 64.6 | 33.6 | 93.6 |
| | | | | | 111.0 | 39.5 | 9.8 | 69.8 |






| | | | | | | | | |
|---------------------|----------|-------|------|--------|-------|------|------|------|
| 1,4-Dichlorobenzene | 134.3028 | 12.12 | 0.00 | 199434 | 148.0 | 64.2 | 33.1 | 93.1 |
| | | | | | 111.0 | 39.3 | 9.1 | 69.1 |




Quantitation Results Report (QT Reviewed)

| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,2-Dichlorobenzene | 136.8411 | 12.49 | 0.00 | 168422 | 148.0 | 62.4 | 33.9 | 93.9 |
| | | | | | 111.0 | 39.9 | 11.0 | 71.0 |



Quantitation Results Report (QT Reviewed)

| | | | |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File | 05JAN27.D | Operator | MSC |
| Acq. Method | 5975CACQF.M | Acq. Date-Time | 1/5/2022 9:55:17 PM |
| Sample Name | CCV010522_Closing | Instrument | VOA5975C |
| Vial | 27 | Multiplier | 1.00 |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m | Comment | |
| Tune File | BFB_Atune3.u | Tune Date | 10/11/2021 4:02:00 PM |
| Batch Name | VG010522_8260B.batch.bin | Last Calib Update | 2/28/2022 2:48:47 PM |
| Ref Library | \\MASSHUNTER\Org\Library\NIST129K.I | | |















| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|--------------------|-------|----------|
| Internal Standards | | | | | | |
| M Fluorobenzene | 6.618 | 96.0 | 792987 | 250.0000 | ng | -0.006 |
| M Chlorobenzene-d5 | 9.774 | 82.0 | 303776 | 250.0000 | ng | 0.003 |
| M 1,4-Dichlorobenzene-d4 | 12.100 | 152.0 | 251051 | 250.0000 | ng | 0.000 |
| System Monitoring Compounds | | | | | | |
| S Dibromofluoromethane | 5.848 | 113.0 | 202444 | 270.9825 | ng | 0.003 |
| Spiked Amount: 250.000 | Range: 80.0 - 119.0% | | | Recovery = 108.39% | | |
| S 1,2-Dichloroethane-d4 | 6.230 | 67.0 | 89848 | 278.4412 | ng | -0.003 |
| Spiked Amount: 250.000 | Range: 81.0 - 118.0% | | | Recovery = 111.38% | | |
| S Toluene-d8 | 8.319 | 98.0 | 805459 | 275.1504 | ng | 0.000 |
| Spiked Amount: 250.000 | Range: 89.0 - 112.0% | | | Recovery = 110.06% | | |
| S p-Bromofluorobenzene | 10.951 | 95.0 | 244993 | 266.3753 | ng | -0.003 |
| Spiked Amount: 250.000 | Range: 85.0 - 114.0% | | | Recovery = 106.55% | | |
| Target Compounds | | | | | | |
| T Dichlorodifluoromethane | 1.244 | 85.0 | 125538 | 120.8077 | ng | 99 |
| T Chloromethane | 1.408 | 50.0 | 147629 | 117.0470 | ng | 99 |
| T Vinyl chloride | 1.500 | 62.0 | 135486 | 119.3808 | ng | 93 |
| T Bromomethane | 1.799 | 96.0 | 62776 | 123.7027 | ng | 97 |
| T Chloroethane | 1.896 | 64.0 | 62102 | 110.5322 | ng | 97 |
| T Trichlorofluoromethane | 2.147 | 101.0 | 173239 | 122.9808 | ng | 99 |
| T 1,1-Dichloroethene | 2.705 | 96.0 | 95980 | 120.1615 | ng | 99 |
| T Methylene chloride | 3.335 | 49.0 | 132759 | 112.7466 | ng | 98 |
| T trans-1,2-Dichloroethene | 3.715 | 96.0 | 99903 | 122.5939 | ng | 98 |
| T Methyl tert-butyl ether (MTBE) | 3.756 | 73.0 | 124004 | 117.7262 | ng | 100 |
| T 1,1-Dichloroethane | 4.378 | 63.0 | 185400 | 122.2257 | ng | 99 |
| T 2,2-Dichloropropane | 5.195 | 77.0 | 135270 | 119.0124 | ng | 99 |
| T cis-1,2-Dichloroethene | 5.212 | 96.0 | 100538 | 121.6867 | ng | 96 |
| T Methyl ethyl ketone | 5.282 | 43.0 | 126386 | 1129.3341 | ng | 98 |
| T Bromochloromethane | 5.519 | 128.0 | 41180 | 120.3132 | ng | 97 |
| T Chloroform | 5.653 | 83.0 | 175506 | 116.2603 | ng | 99 |

Quantitation Results Report (QT Reviewed)

| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|-----------------------------|--------|-------|--------|----------|-------|----------|
| T 1,1,1-Trichloroethane | 5.831 | 97.0 | 171504 | 121.2274 | ng | 99 |
| T Carbon tetrachloride | 6.024 | 117.0 | 169813 | 121.8270 | ng | 98 |
| T 1,1-Dichloropropene | 6.040 | 75.0 | 146239 | 121.5732 | ng | 100 |
| T Benzene | 6.280 | 78.0 | 386868 | 122.5303 | ng | 100 |
| T 1,2-Dichloroethane | 6.319 | 62.0 | 102446 | 119.9409 | ng | 98 |
| T Trichloroethene | 7.028 | 95.0 | 110911 | 121.0621 | ng | 98 |
| T 1,2-Dichloropropane | 7.273 | 63.0 | 93184 | 115.6303 | ng | 98 |
| T Dibromomethane | 7.396 | 93.0 | 40231 | 118.1336 | ng | 95 |
| T Bromodichloromethane | 7.585 | 83.0 | 111872 | 119.0304 | ng | 99 |
| T cis-1,3-Dichloropropene | 8.059 | 75.0 | 120418 | 113.3200 | ng | 97 |
| T Toluene | 8.386 | 92.0 | 240882 | 121.8165 | ng | 99 |
| T trans-1,3-Dichloropropene | 8.637 | 75.0 | 90457 | 119.5883 | ng | 97 |
| T 1,1,2-Trichloroethane | 8.815 | 83.0 | 45451 | 115.3607 | ng | 98 |
| T Tetrachloroethene | 8.938 | 163.8 | 96106 | 119.1324 | ng | 98 |
| T 1,3-Dichloropropane | 8.982 | 76.0 | 91732 | 118.3691 | ng | 98 |
| T Chlorodibromomethane | 9.203 | 129.0 | 72728 | 118.1104 | ng | 99 |
| T 1,2-Dibromoethane | 9.303 | 107.0 | 49436 | 114.7549 | ng | 100 |
| T Chlorobenzene | 9.802 | 112.0 | 261094 | 120.6036 | ng | 99 |
| T 1,1,1,2-Tetrachloroethane | 9.891 | 131.0 | 89675 | 118.4971 | ng | 97 |
| T Ethylbenzene | 9.917 | 91.0 | 453620 | 120.8154 | ng | 99 |
| T m+p-Xylenes | 10.039 | 106.0 | 366259 | 251.0157 | ng | 99 |
| T o-Xylene | 10.432 | 106.0 | 159843 | 123.0566 | ng | 100 |
| T Styrene | 10.446 | 104.0 | 265447 | 126.9277 | ng | 99 |
| T Bromoform | 10.625 | 172.5 | 39014 | 121.4405 | ng | 98 |
| T Bromobenzene | 11.093 | 156.0 | 100992 | 124.3029 | ng | 98 |
| T 1,1,2,2-Tetrachloroethane | 11.116 | 83.0 | 56019 | 119.7931 | ng | 98 |
| T 1,2,3-Trichloropropane | 11.146 | 110.0 | 13841 | 110.6173 | ng | 91 |
| T 2-Chlorotoluene | 11.291 | 126.0 | 101550 | 125.6181 | ng | 97 |
| T 4-Chlorotoluene | 11.400 | 91.0 | 330418 | 125.3600 | ng | 99 |
| T 1,3-Dichlorobenzene | 12.033 | 146.0 | 179363 | 121.0460 | ng | 99 |
| T 1,4-Dichlorobenzene | 12.122 | 146.0 | 177069 | 117.1952 | ng | 96 |
| T 1,2-Dichlorobenzene | 12.493 | 146.0 | 148487 | 118.5734 | ng | 99 |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)

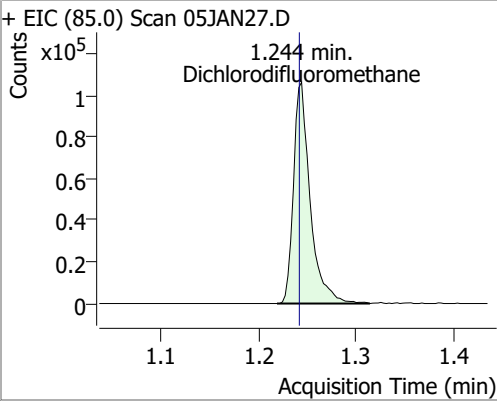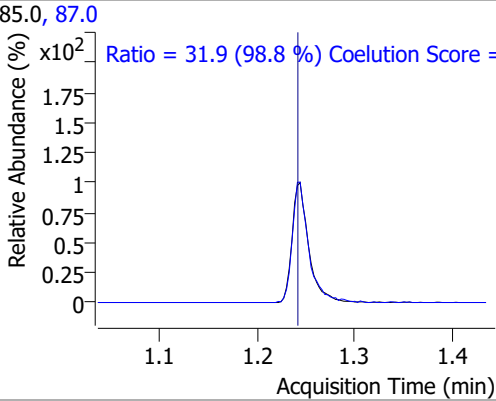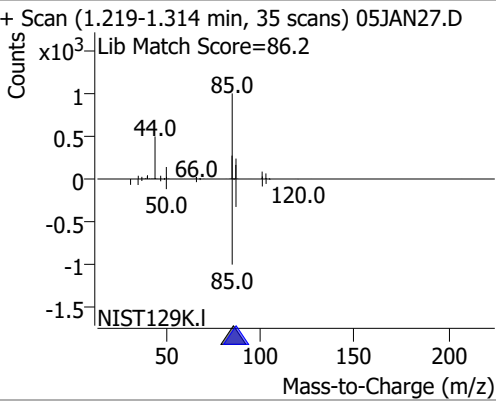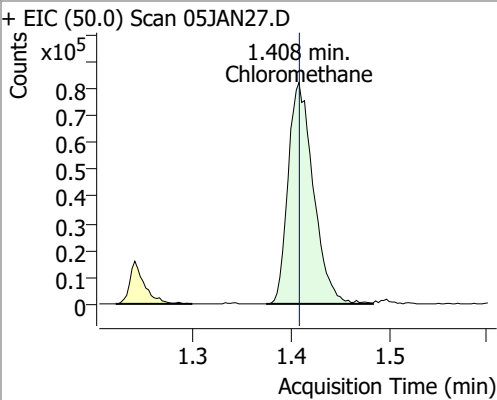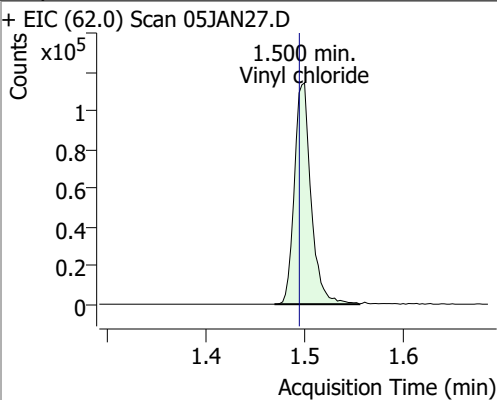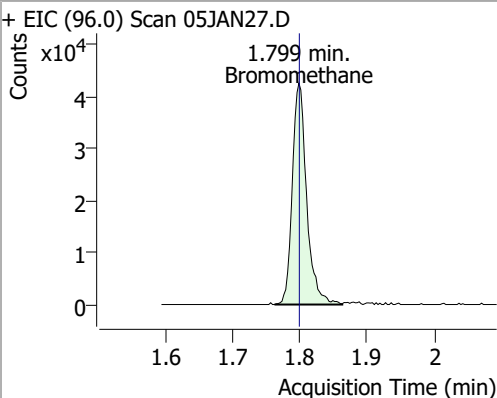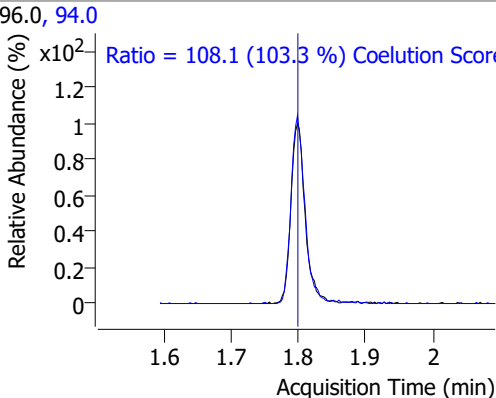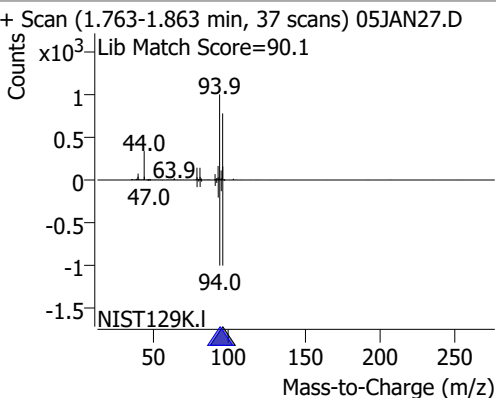
| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---|----------|------|--|--------|------|---|-------|-------|
| Dichlorodifluoromethane | 120.8077 | 1.24 | 0.00 | 125538 | 87.0 | 31.9 | 2.3 | 62.3 |
| + EIC (85.0) Scan 05JAN27.D  | | | 85.0, 87.0  | | | + Scan (1.219-1.314 min, 35 scans) 05JAN27.D Lib Match Score=86.2  | | |
| Chloromethane | 117.0470 | 1.41 | 0.00 | 147629 | 52.0 | 31.7 | 2.1 | 62.1 |
| + EIC (50.0) Scan 05JAN27.D  | | | 50.0, 52.0  | | | + Scan (1.375-1.484 min, 40 scans) 05JAN27.D Lib Match Score=84.9  | | |
| Vinyl chloride | 119.3808 | 1.50 | 0.01 | 135486 | 64.0 | 33.5 | 0.0 | 59.9 |
| + EIC (62.0) Scan 05JAN27.D  | | | 62.0, 64.0  | | | + Scan (1.470-1.556 min, 31 scans) 05JAN27.D Lib Match Score=87.7  | | |
| Bromomethane | 123.7027 | 1.80 | 0.00 | 62776 | 94.0 | 108.1 | 74.6 | 134.6 |
| + EIC (96.0) Scan 05JAN27.D  | | | 96.0, 94.0  | | | + Scan (1.763-1.863 min, 37 scans) 05JAN27.D Lib Match Score=90.1  | | |

Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|----------|------|----------|-------|------|--------|-------|-------|
| Chloroethane | 110.5322 | 1.90 | 0.00 | 62102 | 66.0 | 31.7 | 0.1 | 60.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Trichlorofluoromethane | 122.9808 | 2.15 | 0.01 | 173239 | 103.0 | 63.8 | 34.2 | 94.2 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,1-Dichloroethene | 120.1615 | 2.71 | 0.01 | 95980 | 61.0 | 181.7 | 150.3 | 210.3 |
| | | | | | 63.0 | 57.2 | 26.7 | 86.7 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| Methylene chloride | 112.7466 | 3.34 | 0.00 | 132759 | 84.0 | 66.0 | 36.9 | 96.9 |
| | | | | | 86.0 | 42.9 | 14.3 | 74.3 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------------|----------|------|----------|-------|------|--------|-------|-------|
| trans-1,2-Dichloroethene | 122.5939 | 3.71 | 0.00 | 99903 | 61.0 | 154.4 | 123.9 | 183.9 |
| | | | | | 98.0 | 62.1 | 35.7 | 95.7 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------------------|----------|------|----------|--------|------|--------|-------|-------|
| Methyl tert-butyl ether (MTBE) | 117.7262 | 3.76 | 0.00 | 124004 | 57.0 | 24.8 | 0.0 | 54.6 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1-Dichloroethane | 122.2257 | 4.38 | 0.00 | 185400 | 65.0 | 32.2 | 2.1 | 62.1 |
| | | | | | 83.0 | 13.0 | 0.0 | 43.7 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 2,2-Dichloropropane | 119.0124 | 5.20 | 0.00 | 135270 | 41.0 | 67.2 | 36.5 | 96.5 |
| | | | | | 97.0 | 22.3 | 0.0 | 53.2 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,2-Dichloroethene | 121.6867 | 5.21 | 0.00 | 100538 | 61.0 | 162.0 | 137.2 | 197.2 |
| | | | | | 98.0 | 64.8 | 37.3 | 97.3 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|-----------|------|----------|--------|------|--------|-------|-------|
| Methyl ethyl ketone | 1129.3341 | 5.28 | 0.00 | 126386 | 72.0 | 20.2 | 0.0 | 51.3 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|-------|------|--------|-------|-------|
| Bromochloromethane | 120.3132 | 5.52 | 0.00 | 41180 | 49.0 | 178.1 | 152.9 | 212.9 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|------|--------|-------|-------|
| Chloroform | 116.2603 | 5.65 | 0.00 | 175506 | 85.0 | 65.3 | 36.0 | 96.0 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1,1-Trichloroethane | 121.2274 | 5.83 | 0.00 | 171504 | 99.0 | 66.1 | 34.7 | 94.7 |
| | | | | | 61.0 | 47.8 | 18.1 | 78.1 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Dibromofluoromethane | 270.9825 | 5.85 | 0.00 | 202444 | 191.5 | 22.4 | 0.0 | 53.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Carbon tetrachloride | 121.8270 | 6.02 | 0.00 | 169813 | 119.0 | 95.2 | 67.2 | 127.2 |
| | | | | | 121.0 | 30.7 | 0.1 | 60.1 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|-------|--------|-------|-------|
| 1,1-Dichloropropene | 121.5732 | 6.04 | 0.00 | 146239 | 110.0 | 36.0 | 5.9 | 65.9 |
| | | | | | 77.0 | 30.2 | 0.1 | 60.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 278.4412 | 6.23 | 0.00 | 89848 | 65.0 | 195.0 | 166.5 | 226.5 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|------|----------|--------|------|--------|-------|-------|
| Benzene | 122.5303 | 6.28 | 0.00 | 386868 | 77.0 | 23.7 | 0.0 | 53.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloroethane | 119.9409 | 6.32 | 0.00 | 102446 | 64.0 | 30.8 | 0.0 | 59.9 |
| | | | | | 98.0 | 6.3 | 0.0 | 37.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|----------|------|----------|--------|-------|--------|-------|-------|
| Trichloroethene | 121.0621 | 7.03 | 0.00 | 110911 | 130.0 | 103.3 | 71.5 | 131.5 |
| | | | | | 97.0 | 65.9 | 34.1 | 94.1 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloropropane | 115.6303 | 7.27 | 0.00 | 93184 | 76.0 | 39.7 | 8.2 | 68.2 |






| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------|----------|------|----------|-------|-------|--------|-------|-------|
| Dibromomethane | 118.1336 | 7.40 | 0.00 | 40231 | 173.5 | 106.9 | 83.7 | 143.7 |
| | | | | | 95.0 | 80.4 | 52.2 | 112.2 |






Quantitation Results Report (QT Reviewed)




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Bromodichloromethane | 119.0304 | 7.59 | 0.00 | 111872 | 85.0 | 65.3 | 34.5 | 94.5 |
| | | | | | 127.0 | 9.4 | 0.0 | 39.6 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,3-Dichloropropene | 113.3200 | 8.06 | 0.00 | 120418 | 39.0 | 55.1 | 23.3 | 83.3 |
| | | | | | 77.0 | 32.5 | 1.0 | 61.0 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 275.1504 | 8.32 | 0.00 | 805459 | 100.0 | 63.7 | 34.4 | 94.4 |
| | | | | | 99.0 | 9.7 | 0.0 | 39.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|------|----------|--------|------|--------|-------|-------|
| Toluene | 121.8165 | 8.39 | 0.00 | 240882 | 91.0 | 176.9 | 145.8 | 205.8 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|----------|------|----------|-------|------|--------|-------|-------|
| trans-1,3-Dichloropropene | 119.5883 | 8.64 | 0.00 | 90457 | 39.0 | 49.8 | 23.4 | 83.4 |
| | | | | | 77.0 | 32.4 | 2.4 | 62.4 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,1,2-Trichloroethane | 115.3607 | 8.82 | 0.00 | 45451 | 97.0 | 115.0 | 84.6 | 144.6 |
| | | | | | 85.0 | 64.2 | 37.6 | 97.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------|----------|------|----------|-------|-------|--------|-------|-------|
| Tetrachloroethene | 119.1324 | 8.94 | 0.00 | 96106 | 165.8 | 127.8 | 98.6 | 158.6 |
| | | | | | 129.0 | 89.0 | 61.5 | 121.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,3-Dichloropropane | 118.3691 | 8.98 | 0.00 | 91732 | 78.0 | 32.0 | 2.9 | 62.9 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|------|----------|-------|-------|--------|-------|-------|
| Chlorodibromomethane | 118.1104 | 9.20 | 0.00 | 72728 | 127.0 | 77.1 | 48.0 | 108.0 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------|----------|------|----------|-------|-------|--------|-------|-------|
| 1,2-Dibromoethane | 114.7549 | 9.30 | 0.00 | 49436 | 109.0 | 94.6 | 64.5 | 124.5 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------|----------|------|----------|--------|-------|--------|-------|-------|
| Chlorobenzene | 120.6036 | 9.80 | 0.00 | 261094 | 114.0 | 32.5 | 2.1 | 62.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|----------|------|----------|-------|-------|--------|-------|-------|
| 1,1,1,2-Tetrachloroethane | 118.4971 | 9.89 | 0.00 | 89675 | 133.0 | 95.9 | 68.6 | 128.6 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|----------|------|----------|--------|-------|--------|-------|-------|
| Ethylbenzene | 120.8154 | 9.92 | 0.00 | 453620 | 106.0 | 31.6 | 1.1 | 61.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------|----------|-------|----------|--------|------|--------|-------|-------|
| m+p-Xylenes | 251.0157 | 10.04 | 0.00 | 366259 | 91.0 | 199.4 | 171.4 | 231.4 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|-------|----------|--------|------|--------|-------|-------|
| o-Xylene | 123.0566 | 10.43 | 0.00 | 159843 | 91.0 | 212.7 | 183.1 | 243.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|----------|-------|----------|--------|------|--------|-------|-------|
| Styrene | 126.9277 | 10.45 | 0.00 | 265447 | 78.0 | 49.1 | 19.6 | 79.6 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------|----------|-------|----------|-------|-------|--------|-------|-------|
| Bromoform | 121.4405 | 10.62 | 0.00 | 39014 | 170.5 | 51.6 | 22.1 | 82.1 |
| | | | | | 174.5 | 48.2 | 20.1 | 80.1 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 266.3753 | 10.95 | 0.00 | 244993 | 174.0 | 94.6 | 61.7 | 121.7 |
| | | | | | 176.0 | 90.0 | 60.6 | 120.6 |




Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|----------|-------|----------|--------|-------|--------|-------|-------|
| Bromobenzene | 124.3029 | 11.09 | 0.00 | 100992 | 77.0 | 142.9 | 115.7 | 175.7 |
| | | | | | 158.0 | 97.8 | 66.5 | 126.5 |




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|----------|-------|----------|-------|------|--------|-------|-------|
| 1,1,2,2-Tetrachloroethane | 119.7931 | 11.12 | 0.00 | 56019 | 85.0 | 64.9 | 36.2 | 96.2 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|----------|-------|----------|-------|-------|--------|-------|-------|
| 1,2,3-Trichloropropane | 110.6173 | 11.15 | 0.00 | 13841 | 112.0 | 70.2 | 33.5 | 93.5 |






| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|----------|-------|----------|--------|------|--------|-------|-------|
| 2-Chlorotoluene | 125.6181 | 11.29 | 0.00 | 101550 | 91.0 | 277.1 | 252.3 | 312.3 |






Quantitation Results Report (QT Reviewed)




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 4-Chlorotoluene | 125.3600 | 11.40 | 0.00 | 330418 | 126.0 | 32.2 | 1.7 | 61.7 |



| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,3-Dichlorobenzene | 121.0460 | 12.03 | 0.00 | 179363 | 148.0 | 63.5 | 33.6 | 93.6 |
| | | | | | 111.0 | 38.6 | 9.8 | 69.8 |






| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,4-Dichlorobenzene | 117.1952 | 12.12 | 0.00 | 177069 | 148.0 | 66.5 | 33.1 | 93.1 |
| | | | | | 111.0 | 40.6 | 9.1 | 69.1 |



Quantitation Results Report (QT Reviewed)

| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,2-Dichlorobenzene | 118.5734 | 12.49 | 0.00 | 148487 | 148.0 | 64.3 | 33.9 | 93.9 |
| | | | | | 111.0 | 39.4 | 11.0 | 71.0 |



Audit Trail report

Batch name and path: D:\Org\Data\VOA5975C\VG010522\QuantResults\VG010522_8260B.batch.bin
Quant batch version: 10.0
Quant reporting version: 10.0

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|------------------------------|----------------|----------------------|---|--------|---------|---------|-----------|
| CmdNewBatchTable | BL2000\mchavez | 1/5/2022 10:06:32 AM | Create new batch D:\Org\Data\VOA5975C\VG010522\VG010522_8260B.batch.bin | | | ✓ | |
| CmdImportSamplesFromWorklist | BL2000\mchavez | 1/5/2022 10:06:44 AM | Add samples from worklist: D:\Org\Data\VOA5975C\VG010522\05JAN02.D, D:\Org\Data\VOA5975C\VG010522\05JAN01.D | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 10:09:25 AM | Set SampleType = TuneCheck for sample 05JAN02.D; previous value = Sample | | | ✓ | |
| CmdSaveBatchTable | BL2000\mchavez | 1/5/2022 10:09:53 AM | Save batch D:\Org\Data\VOA5975C\VG010522\QuantResults\VG010522_8260B.batch.bin | | | ✓ | |
| CmdOpenBatchTable | BL2000\mchavez | 1/5/2022 11:08:02 AM | Open batch D:\Org\Data\VOA5975C\VG010522\VG010522_8260B.batch.bin | | | ✓ | |
| CmdImportSamplesFromWorklist | BL2000\mchavez | 1/5/2022 11:08:14 AM | Add samples from worklist: D:\Org\Data\VOA5975C\VG010522\05JAN03.D | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 11:08:17 AM | Set SampleType = CC for sample 05JAN03.D; previous value = Sample | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 11:08:21 AM | Set LevelName = CC for sample 05JAN03.D; previous value = | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/5/2022 11:08:23 AM | Quantitate all compounds in all samples | | | ✓ | |
| CmdStartMethodEditing | BL2000\mchavez | 1/5/2022 11:08:36 AM | Start method editing | | | ✓ | |
| CmdImportMethodFromBatch | BL2000\mchavez | 1/5/2022 11:08:37 AM | Import method from batch D:\Org\Data\VOA5977B\VH010422\VH010422_8260B_624pt1.batch.bin | | | ✓ | |
| CmdMethodClear | BL2000\mchavez | 1/5/2022 11:08:56 AM | Clear method | | | ✓ | |
| CmdImportMethodFromBatch | BL2000\mchavez | 1/5/2022 11:08:58 AM | Import method from batch D:\Org\Data\VOA5975C\VG010422\VG010422_8260B.batch.bin | | | ✓ | |
| CmdApplyMethodToAllSamples | BL2000\mchavez | 1/5/2022 11:09:02 AM | Apply method to all samples | | | ✓ | |
| CmdMethodClear | BL2000\mchavez | 1/5/2022 11:09:02 AM | Clear method | | | ✓ | |
| CmdEndMethodEditing | BL2000\mchavez | 1/5/2022 11:09:02 AM | End method editing | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/5/2022 11:09:07 AM | Quantitate all compounds in all samples | | | ✓ | |
| CmdImportSamplesFromWorklist | BL2000\mchavez | 1/5/2022 11:46:31 AM | Add samples from worklist: D:\Org\Data\VOA5975C\VG010522\05JAN04.D | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 11:46:35 AM | Set SampleType = QC for sample 05JAN04.D; previous value = Sample | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|------------------------------|----------------|----------------------|---|--------|---------|---------|-----------|
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 11:46:40 AM | Set LevelName = QC for sample 05JAN04.D; previous value = | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 11:46:46 AM | Set SampleInformation = LCSA for sample 05JAN04.D; previous value = | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/5/2022 11:46:50 AM | Quantitate all compounds in all samples | | | ✓ | |
| CmdSaveBatchTable | BL2000\mchavez | 1/5/2022 12:10:46 PM | Save batch D:\Org\Data\VOA5975C\VG010522\QuantResults\VG010522_8260B.batch.bin | | | ✓ | |
| CmdOpenBatchTable | BL2000\mchavez | 1/5/2022 12:40:50 PM | Open batch D:\Org\Data\VOA5975C\VG010522\VG010522_8260B.batch.bin | | | ✓ | |
| CmdImportSamplesFromWorklist | BL2000\mchavez | 1/5/2022 12:41:18 PM | Add samples from worklist: D:\Org\Data\VOA5975C\VG010522\05JAN06.D, D:\Org\Data\VOA5975C\VG010522\05JAN05.D | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 12:41:28 PM | Set SampleType = Blank for sample 05JAN06.D; previous value = Sample | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/5/2022 12:41:33 PM | Quantitate all compounds in all samples | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/5/2022 12:42:20 PM | Quantitate all compounds in all samples | | | ✓ | |
| CmdSaveBatchTable | BL2000\mchavez | 1/5/2022 12:42:58 PM | Save batch D:\Org\Data\VOA5975C\VG010522\QuantResults\VG010522_8260B.batch.bin | | | ✓ | |
| CmdOpenBatchTable | BL2000\mchavez | 1/5/2022 2:33:02 PM | Open batch D:\Org\Data\VOA5975C\VG010522\VG010522_8260B.batch.bin | | | ✓ | |
| CmdImportSamplesFromWorklist | BL2000\mchavez | 1/5/2022 2:33:41 PM | Add samples from worklist: D:\Org\Data\VOA5975C\VG010522\05JAN09.D, D:\Org\Data\VOA5975C\VG010522\05JAN08.D, D:\Org\Data\VOA5975C\VG010522\05JAN07.D | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/5/2022 2:33:49 PM | Quantitate all compounds in all samples | | | ✓ | |
| CmdImportSamplesFromWorklist | BL2000\mchavez | 1/5/2022 2:36:55 PM | Add samples from worklist: D:\Org\Data\VOA5975C\VG010522\05JAN10.D | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/5/2022 2:37:06 PM | Quantitate all compounds in all samples | | | ✓ | |
| CmdStartMethodEditing | BL2000\mchavez | 1/5/2022 2:44:33 PM | Start method editing | | | ✓ | |
| CmdImportMethodFromSample | BL2000\mchavez | 1/5/2022 2:44:34 PM | Import method from sample 05JAN10.D | | | ✓ | |
| CmdApplyMethodToAllSamples | BL2000\mchavez | 1/5/2022 2:47:34 PM | Apply method to all samples | | | ✓ | |
| CmdMethodClear | BL2000\mchavez | 1/5/2022 2:47:35 PM | Clear method | | | ✓ | |
| CmdEndMethodEditing | BL2000\mchavez | 1/5/2022 2:47:36 PM | End method editing | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|---------------------|---|--------|---------|---------|-----------|
| CmdQuantitate | BL2000\mchavez | 1/5/2022 2:47:41 PM | Quantitate all compounds in all samples | | | ✓ | |
| CmdImportSamplesFromWorklist | BL2000\mchavez | 1/5/2022 3:02:57 PM | Add samples from worklist: D:\Org\Data\VOA5975C\VG010522\05JAN11.D | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/5/2022 3:03:07 PM | Quantitate all compounds in all samples | | | ✓ | |
| CmdSaveBatchTable | BL2000\mchavez | 1/5/2022 3:04:23 PM | Save batch D:\Org\Data\VOA5975C\VG010522\QuantResults\VG010522_8260B.batch.bin | | | ✓ | |
| CmdOpenBatchTable | BL2000\mchavez | 1/5/2022 3:32:09 PM | Open batch D:\Org\Data\VOA5975C\VG010522\VG010522_8260B.batch.bin | | | ✓ | |
| CmdImportSamplesFromWorklist | BL2000\mchavez | 1/5/2022 3:32:24 PM | Add samples from worklist: D:\Org\Data\VOA5975C\VG010522\05JAN12.D | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/5/2022 3:32:32 PM | Quantitate all compounds in all samples | | | ✓ | |
| CmdSaveBatchTable | BL2000\mchavez | 1/5/2022 4:00:06 PM | Save batch D:\Org\Data\VOA5975C\VG010522\QuantResults\VG010522_8260B.batch.bin | | | ✓ | |
| CmdOpenBatchTable | BL2000\mchavez | 1/5/2022 4:37:21 PM | Open batch D:\Org\Data\VOA5975C\VG010522\VG010522_8260B.batch.bin | | | ✓ | |
| CmdImportSamplesFromWorklist | BL2000\mchavez | 1/5/2022 4:37:49 PM | Add samples from worklist: D:\Org\Data\VOA5975C\VG010522\05JAN14.D, D:\Org\Data\VOA5975C\VG010522\05JAN13.D | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/5/2022 4:38:00 PM | Quantitate all compounds in all samples | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 4:38:36 PM | Manually integrate compound Chlorodibromomethane in sample 05JAN14.D, from x, y = 9.169, 0 to 9.233, 0, result = 3282; previous integration is from x, y = 9.194, 0 to 9.233, 0 and previous response = 2357. | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 4:38:54 PM | Manually integrate compound Chloroform in sample 05JAN14.D, from x, y = 5.597, 0 to 5.706, 0, result = 2570; previous integration is from x, y = 5.636, 0 to 5.689, 0 and previous response = 2109. | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 4:38:57 PM | Manually integrate qualifier 85.0 of compound Chloroform in sample 05JAN14.D from x, y = 5.611, 0 to 5.706, 0; result = 1771 | | | ✓ | |
| CmdZeroOutPeak | BL2000\mchavez | 1/5/2022 4:39:08 PM | Zero out primary peak of compound 4-Chlorotoluene in sample 05JAN14.D | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|------------------------------|----------------|---------------------|---|--------|---------|---------|-----------|
| CmdSaveBatchTable | BL2000\mchavez | 1/5/2022 4:55:15 PM | Save batch D:\Org\Data\VOA5975C\VG010522\QuantResults\VG010522_8260B.batch.bin | | | ✓ | |
| CmdOpenBatchTable | BL2000\mchavez | 1/6/2022 8:31:32 AM | Open batch D:\Org\Data\VOA5975C\VG010522\VG010522_8260B.batch.bin | | | ✓ | |
| CmdImportSamplesFromWorklist | BL2000\mchavez | 1/6/2022 8:33:55 AM | Add samples from worklist: D:\Org\Data\VOA5975C\VG010522\05JAN29.D, D:\Org\Data\VOA5975C\VG010522\05JAN28.D, D:\Org\Data\VOA5975C\VG010522\05JAN27.D, D:\Org\Data\VOA5975C\VG010522\05JAN26.D, D:\Org\Data\VOA5975C\VG010522\05JAN25.D, D:\Org\Data\VOA5975C\VG010522\05JAN24.D, D:\Org\Data\VOA5975C\VG010522\05JAN23.D, D:\Org\Data\VOA5975C\VG010522\05JAN22.D, D:\Org\Data\VOA5975C\VG010522\05JAN21.D, D:\Org\Data\VOA5975C\VG010522\05JAN20.D, D:\Org\Data\VOA5975C\VG010522\05JAN19.D, D:\Org\Data\VOA5975C\VG010522\05JAN18.D, D:\Org\Data\VOA5975C\VG010522\05JAN17.D, D:\Org\Data\VOA5975C\VG010522\05JAN16.D, D:\Org\Data\VOA5975C\VG010522\05JAN15.D | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/6/2022 8:34:07 AM | Set SampleType = CC for sample 05JAN27.D; previous value = Sample | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/6/2022 8:34:16 AM | Set LevelName = CC for sample 05JAN27.D; previous value = | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/6/2022 8:34:21 AM | Set SampleType = Matrix for sample 05JAN24.D; previous value = Sample | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/6/2022 8:34:26 AM | Set SampleType = MatrixDup for sample 05JAN25.D; previous value = Sample | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/6/2022 8:36:48 AM | Set SampleInformation = MatrixA for sample 05JAN24.D; previous value = | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/6/2022 8:36:52 AM | Set SampleInformation = MatrixA for sample 05JAN25.D; previous value = | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/6/2022 8:37:11 AM | Quantitate all compounds in all samples | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/6/2022 8:37:19 AM | Set MatrixSpikeGroup = 2 for sample 05JAN24.D; previous value = | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|-----------------------|---|--------|---------|---------|-----------|
| CmdSetSampleAttribute | BL2000\mchavez | 1/6/2022 8:37:23 AM | Set MatrixSpikeGroup = 2 for sample 05JAN25.D; previous value = | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/6/2022 8:37:30 AM | Set MatrixSpikeGroup = 2 for sample 05JAN14.D; previous value = | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/6/2022 8:37:50 AM | Quantitate all compounds in all samples | | | ✓ | |
| CmdSaveBatchTable | BL2000\mchavez | 1/6/2022 10:07:46 AM | Save batch D:\Org\Data\VOA5975C\VG010522\QuantResults\VG010522_8260B.batch.bin | | | ✓ | |
| CmdOpenBatchTable | BL2000\mchavez | 1/9/2022 9:04:24 PM | Open batch D:\Org\Data\VOA5975C\VG010522\VG010522_8260B.batch.bin | | | ✓ | |
| CmdStartMethodEditing | BL2000\mchavez | 1/9/2022 9:05:13 PM | Start method editing | | | ✓ | |
| CmdImportMethodFrom File | BL2000\mchavez | 1/9/2022 9:05:14 PM | Import method from file \\MASSHUNTER\Org\Data\Methods\Quant\VOA5975C\VOA5975C_010422_CAL\VOA5975C_8260B_SHT_DoD_L4_010422.m | | | ✓ | |
| CmdApplyMethodToAllSamples | BL2000\mchavez | 1/9/2022 9:05:27 PM | Apply method to all samples | | | ✓ | |
| CmdMethodClear | BL2000\mchavez | 1/9/2022 9:05:27 PM | Clear method | | | ✓ | |
| CmdEndMethodEditing | BL2000\mchavez | 1/9/2022 9:05:27 PM | End method editing | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/9/2022 9:05:41 PM | Quantitate all compounds in all samples | | | ✓ | |
| CmdSaveBatchTable | BL2000\mchavez | 1/9/2022 9:06:14 PM | Save batch D:\Org\Data\VOA5975C\VG010522\QuantResults\VG010522_8260B.batch.bin | | | ✓ | |
| CmdOpenBatchTable | BL2000\mchavez | 1/10/2022 12:44:09 PM | Open batch D:\Org\Data\VOA5975C\VG010522\VG010522_8260B.batch.bin | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 12:44:18 PM | Set SampleApproved = True for sample 05JAN02.D; previous value = False | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 12:47:41 PM | Set SampleApproved = True for sample 05JAN03.D; previous value = False | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 12:48:32 PM | Set SampleApproved = True for sample 05JAN04.D; previous value = False | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 12:48:58 PM | Manually integrate compound Methylene chloride in sample 05JAN06.D from x, y = 3.282, 0 to 3.377, 0; result = 1656 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 12:49:00 PM | Manually integrate qualifier 84.0 of compound Methylene chloride in sample 05JAN06.D from x, y = 3.294, 0 to 3.391, 0; result = 783 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 12:49:05 PM | Manually integrate qualifier 86.0 of compound Methylene chloride in sample 05JAN06.D from x, y = 3.277, 0 to 3.386, 0; result = 764 | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|-----------------------|---|--------|---------|---------|-----------|
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 12:49:09 PM | Set UserAnnotation = NI for compound Methylene chloride in sample 05JAN06.D; previous value = | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 12:50:50 PM | Set SampleApproved = True for sample 05JAN06.D; previous value = False | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 12:51:41 PM | Manually integrate compound Toluene in sample 05JAN07.D from x, y = 8.349, 0 to 8.422, 0; result = 1710 | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 12:51:45 PM | Set UserAnnotation = NI for compound Toluene in sample 05JAN07.D; previous value = | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 12:52:02 PM | Manually integrate compound Benzene in sample 05JAN07.D from x, y = 6.250, 0 to 6.300, 0; result = 306 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 12:52:06 PM | Manually integrate qualifier 77.0 of compound Benzene in sample 05JAN07.D from x, y = 6.269, 0 to 6.300, 0; result = 56 | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 12:52:12 PM | Set UserAnnotation = NI for compound Benzene in sample 05JAN07.D; previous value = | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 12:52:32 PM | Manually integrate compound Methylene chloride in sample 05JAN07.D from x, y = 3.285, 0 to 3.386, 0; result = 1563 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 12:52:35 PM | Manually integrate qualifier 84.0 of compound Methylene chloride in sample 05JAN07.D from x, y = 3.294, 0 to 3.377, 0; result = 950 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 12:52:38 PM | Manually integrate qualifier 86.0 of compound Methylene chloride in sample 05JAN07.D from x, y = 3.294, 0 to 3.374, 0; result = 316 | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 12:52:42 PM | Set UserAnnotation = NI for compound Methylene chloride in sample 05JAN07.D; previous value = | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 12:52:56 PM | Manually integrate compound Chloromethane in sample 05JAN07.D from x, y = 1.378, 0 to 1.425, 0; result = 579 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 12:53:01 PM | Manually integrate qualifier 52.0 of compound Chloromethane in sample 05JAN07.D from x, y = 1.375, 0 to 1.434, 0; result = 64 | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 12:53:05 PM | Set UserAnnotation = NI for compound Chloromethane in sample 05JAN07.D; previous value = | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 12:53:22 PM | Set SampleApproved = True for sample 05JAN07.D; previous value = False | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|-----------------------|---|--------|---------|---------|-----------|
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 12:54:07 PM | Manually integrate qualifier52.0 of compound Chloromethane in sample 05JAN08.D from x, y = 1.367, 0 to 1.447, 0; result = 1467 | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 12:54:20 PM | Manually integrate compound Methylene chloride in sample 05JAN08.D from x, y = 3.280, 0 to 3.405, 0; result = 1786 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 12:54:22 PM | Manually integrate qualifier84.0 of compound Methylene chloride in sample 05JAN08.D from x, y = 3.299, 0 to 3.394, 0; result = 1069 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 12:54:25 PM | Manually integrate qualifier86.0 of compound Methylene chloride in sample 05JAN08.D from x, y = 3.285, 0 to 3.388, 0; result = 617 | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 12:54:48 PM | Manually integrate compound Toluene in sample 05JAN08.D from x, y = 8.349, 0 to 8.413, 0; result = 1683 | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 12:54:52 PM | Set UserAnnotation = NI for compound Toluene in sample 05JAN08.D; previous value = | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 12:55:16 PM | Set SampleApproved = True for sample 05JAN08.D; previous value = False | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 12:55:23 PM | Set UserAnnotation = NI for compound Methylene chloride in sample 05JAN08.D; previous value = | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 12:55:33 PM | Manually integrate compound Toluene in sample 05JAN09.D from x, y = 8.361, 0 to 8.413, 0; result = 1481 | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 12:55:37 PM | Set UserAnnotation = NI for compound Toluene in sample 05JAN09.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 12:55:44 PM | Set UserAnnotation = for compound Toluene in sample 05JAN09.D; previous value = NI | | | ✓ | |
| CmdZeroOutPeak | BL2000\mchavez | 1/10/2022 12:55:47 PM | Zero out primary peak of compound Toluene in sample 05JAN09.D | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 12:56:18 PM | Set UserDefined = Qualifier ratio did not meet method criteria for Toluene for sample 05JAN09.D; previous value = | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 12:56:22 PM | Manually integrate compound Methylene chloride in sample 05JAN09.D from x, y = 3.296, 0 to 3.383, 0; result = 1869 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 12:56:26 PM | Manually integrate qualifier84.0 of compound Methylene chloride in sample 05JAN09.D from x, y = 3.288, 0 to 3.372, 0; result = 1107 | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|-----------------------|--|--------|---------|---------|-----------|
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 12:56:28 PM | Manually integrate qualifier86.0 of compound Methylene chloride in sample 05JAN09.D from x, y = 3.282, 0 to 3.400, 0; result = 742 | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 12:56:40 PM | Set UserAnnotation = NI for compound Methylene chloride in sample 05JAN09.D; previous value = | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 12:57:49 PM | Manually integrate qualifier52.0 of compound Chloromethane in sample 05JAN09.D from x, y = 1.372, 0 to 1.464, 0; result = 1625 | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 12:57:53 PM | Set SampleApproved = True for sample 05JAN09.D; previous value = False | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/10/2022 12:58:24 PM | Quantitate all compounds in all samples | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 12:58:43 PM | Manually integrate compound Methylene chloride in sample 05JAN10.D from x, y = 3.280, 0 to 3.369, 0; result = 1248 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 12:58:47 PM | Manually integrate qualifier84.0 of compound Methylene chloride in sample 05JAN10.D from x, y = 3.285, 0 to 3.369, 0; result = 681 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 12:58:51 PM | Manually integrate qualifier86.0 of compound Methylene chloride in sample 05JAN10.D from x, y = 3.296, 0 to 3.394, 0; result = 397 | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 12:58:54 PM | Set UserAnnotation = NI for compound Methylene chloride in sample 05JAN10.D; previous value = | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 12:58:59 PM | Manually integrate compound Toluene in sample 05JAN10.D from x, y = 8.349, 0 to 8.428, 0; result = 1581 | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 12:59:04 PM | Set UserAnnotation = NI for compound Toluene in sample 05JAN10.D; previous value = | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 12:59:11 PM | Manually integrate compound Chloromethane in sample 05JAN10.D from x, y = 1.370, 0 to 1.448, 0; result = 1273 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 12:59:14 PM | Manually integrate qualifier52.0 of compound Chloromethane in sample 05JAN10.D from x, y = 1.381, 0 to 1.456, 0; result = 512 | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:02:09 PM | Manually integrate compound m+p-Xylenes in sample 05JAN10.D from x, y = 10.012, 0 to 10.056, 0; result = 169 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:02:13 PM | Manually integrate qualifier91.0 of compound m+p-Xylenes in sample 05JAN10.D from x, y = 10.025, 0 to 10.059, 0; result = 230 | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|--|--------|---------|---------|-----------|
| CmdZeroOutPeak | BL2000\mchavez | 1/10/2022 1:02:16 PM | Zero out primary peak of compound m+p-Xylenes in sample 05JAN10.D | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 1:02:29 PM | Set UserDefined = Qualifier ratio did not meet method criteria for Toluene for sample 05JAN10.D; previous value = | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 1:02:58 PM | Set UserDefined = Qualifier ratio did not meet method criteria for m+p Xylenes for sample 05JAN10.D; previous value = Qualifier ratio did not meet method criteria for Toluene | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 1:03:18 PM | Set SampleApproved = True for sample 05JAN10.D; previous value = False | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:04:00 PM | Manually integrate compound m+p-Xylenes in sample 05JAN11.D from x, y = 10.017, 0 to 10.059, 0; result = 36 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:04:03 PM | Manually integrate qualifier91.0 of compound m+p-Xylenes in sample 05JAN11.D from x, y = 10.011, 0 to 10.073, 0; result = 300 | | | ✓ | |
| CmdZeroOutPeak | BL2000\mchavez | 1/10/2022 1:04:06 PM | Zero out primary peak of compound m+p-Xylenes in sample 05JAN11.D | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 1:04:24 PM | Set UserDefined = Qualifier ratio did not meet method criteria for m+p Xylenes for sample 05JAN11.D; previous value = | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:04:54 PM | Manually integrate compound Benzene in sample 05JAN11.D from x, y = 6.238, 0 to 6.319, 0; result = 424 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:04:57 PM | Manually integrate qualifier77.0 of compound Benzene in sample 05JAN11.D from x, y = 6.241, 0 to 6.319, 0; result = 84 | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 1:05:02 PM | Set UserAnnotation = NI for compound Benzene in sample 05JAN11.D; previous value = | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:05:14 PM | Manually integrate compound Chloroform in sample 05JAN11.D from x, y = 5.622, 0 to 5.686, 0; result = 66 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:05:17 PM | Manually integrate qualifier85.0 of compound Chloroform in sample 05JAN11.D from x, y = 5.625, 0 to 5.681, 0; result = 75 | | | ✓ | |
| CmdZeroOutPeak | BL2000\mchavez | 1/10/2022 1:05:23 PM | Zero out primary peak of compound Chloroform in sample 05JAN11.D | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 1:05:42 PM | Set UserDefined = Qualifier ratio did not meet method criteria for m+p Xylenes, Chloroform for sample 05JAN11.D; previous value = Qualifier ratio did not meet method criteria for m+p Xylenes | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|---|--------|---------|---------|-----------|
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:06:09 PM | Manually integrate compound Methylene chloride in sample 05JAN11.D from x, y = 3.283, 0 to 3.375, 0; result = 1663 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:06:14 PM | Manually integrate qualifier84.0 of compound Methylene chloride in sample 05JAN11.D from x, y = 3.291, 0 to 3.411, 0; result = 1278 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:06:16 PM | Manually integrate qualifier86.0 of compound Methylene chloride in sample 05JAN11.D from x, y = 3.283, 0 to 3.422, 0; result = 795 | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 1:06:22 PM | Set UserAnnotation = NI for compound Methylene chloride in sample 05JAN11.D; previous value = | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:06:36 PM | Manually integrate compound Chloromethane in sample 05JAN11.D from x, y = 1.372, 0 to 1.442, 0; result = 1466 | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 1:06:38 PM | Set UserAnnotation = NI for compound Chloromethane in sample 05JAN11.D; previous value = | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:06:41 PM | Manually integrate qualifier52.0 of compound Chloromethane in sample 05JAN11.D from x, y = 1.353, 0 to 1.453, 0; result = 404 | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/10/2022 1:07:18 PM | Quantitate all compounds in all samples | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 1:07:29 PM | Set SampleApproved = True for sample 05JAN11.D; previous value = False | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:07:51 PM | Manually integrate qualifier84.0 of compound Methylene chloride in sample 05JAN12.D from x, y = 3.294, 0 to 3.375, 0; result = 1439 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:07:53 PM | Manually integrate qualifier86.0 of compound Methylene chloride in sample 05JAN12.D from x, y = 3.305, 0 to 3.377, 0; result = 950 | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:08:09 PM | Manually integrate compound Chloromethane in sample 05JAN12.D from x, y = 1.375, 0 to 1.442, 0; result = 1581 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:08:13 PM | Manually integrate qualifier52.0 of compound Chloromethane in sample 05JAN12.D from x, y = 1.378, 0 to 1.434, 0; result = 426 | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 1:08:17 PM | Set UserAnnotation = NI for compound Chloromethane in sample 05JAN12.D; previous value = | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|---|--------|---------|---------|-----------|
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:08:33 PM | Manually integrate compound Methyl tert-butyl ether (MTBE) in sample 05JAN12.D from x, y = 3.731, 0 to 3.784, 0; result = 28 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:08:36 PM | Manually integrate qualifier 57.0 of compound Methyl tert-butyl ether (MTBE) in sample 05JAN12.D from x, y = 3.743, 0 to 3.784, 0; result = 28 | | | ✓ | |
| CmdZeroOutPeak | BL2000\mchavez | 1/10/2022 1:08:40 PM | Zero out primary peak of compound Methyl tert-butyl ether (MTBE) in sample 05JAN12.D | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 1:08:57 PM | Set UserDefined = Qualifier ratio did not meet method criteria for m+p Xylenes, Chloroform for sample 05JAN12.D; previous value = | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 1:09:16 PM | Set UserDefined = Qualifier ratio did not meet method criteria for MtBE for sample 05JAN12.D; previous value = Qualifier ratio did not meet method criteria for m+p Xylenes, Chloroform | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:10:54 PM | Manually integrate compound Chloroform in sample 05JAN12.D from x, y = 5.614, 0 to 5.692, 0; result = 227 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:10:57 PM | Manually integrate qualifier 85.0 of compound Chloroform in sample 05JAN12.D from x, y = 5.633, 0 to 5.681, 0; result = 28 | | | ✓ | |
| CmdZeroOutPeak | BL2000\mchavez | 1/10/2022 1:11:00 PM | Zero out primary peak of compound Chloroform in sample 05JAN12.D | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 1:11:17 PM | Set UserDefined = Qualifier ratio did not meet method criteria for MtBE, Chloroform for sample 05JAN12.D; previous value = Qualifier ratio did not meet method criteria for MtBE | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:11:39 PM | Manually integrate compound Benzene in sample 05JAN12.D from x, y = 6.241, 0 to 6.333, 0; result = 411 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:11:42 PM | Manually integrate qualifier 77.0 of compound Benzene in sample 05JAN12.D from x, y = 6.241, 0 to 6.317, 0; result = 70 | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 1:12:16 PM | Set SampleApproved = True for sample 05JAN12.D; previous value = False | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:13:06 PM | Manually integrate compound Methylene chloride in sample 05JAN13.D from x, y = 3.282, 0 to 3.372, 0; result = 1841 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:13:09 PM | Manually integrate qualifier 84.0 of compound Methylene chloride in sample 05JAN13.D from x, y = 3.274, 0 to 3.391, 0; result = 1473 | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|--|--------|---------|---------|-----------|
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:13:11 PM | Manually integrate qualifier86.0 of compound Methylene chloride in sample 05JAN13.D from x, y = 3.291, 0 to 3.397, 0; result = 726 | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 1:13:14 PM | Set UserAnnotation = NI for compound Methylene chloride in sample 05JAN13.D; previous value = | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:13:26 PM | Manually integrate compound Chloromethane in sample 05JAN13.D from x, y = 1.383, 0 to 1.431, 0; result = 955 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:13:29 PM | Manually integrate qualifier52.0 of compound Chloromethane in sample 05JAN13.D from x, y = 1.375, 0 to 1.456, 0; result = 206 | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 1:13:35 PM | Set SampleApproved = True for sample 05JAN13.D; previous value = False | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 1:13:46 PM | Set UserAnnotation = NI for compound Chloromethane in sample 05JAN13.D; previous value = | | | ✓ | |
| CmdSaveBatchTable | BL2000\mchavez | 1/10/2022 1:13:49 PM | Save batch D:\Org\Data\VOA5975C\VG010522\QuantResults\VG010522_8260B.batch.bin | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 1:16:16 PM | Set UserAnnotation = NI for compound Chloroform in sample 05JAN14.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 1:16:22 PM | Set UserAnnotation = LT for compound Chloroform in sample 05JAN14.D; previous value = NI | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 1:16:31 PM | Set UserAnnotation = LT for compound Chlorodibromomethane in sample 05JAN14.D; previous value = | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:16:47 PM | Manually integrate compound Chloromethane in sample 05JAN14.D from x, y = 1.386, 0 to 1.456, 0; result = 612 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:16:49 PM | Manually integrate qualifier52.0 of compound Chloromethane in sample 05JAN14.D from x, y = 1.389, 0 to 1.448, 0; result = 152 | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 1:16:55 PM | Set UserAnnotation = NI for compound Chloromethane in sample 05JAN14.D; previous value = | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:17:08 PM | Manually integrate compound Methylene chloride in sample 05JAN14.D from x, y = 3.296, 0 to 3.386, 0; result = 858 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:17:11 PM | Manually integrate qualifier84.0 of compound Methylene chloride in sample 05JAN14.D from x, y = 3.299, 0 to 3.380, 0; result = 344 | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|---|--------|---------|---------|-----------|
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:17:13 PM | Manually integrate qualifier86.0 of compound Methylene chloride in sample 05JAN14.D from x, y = 3.299, 0 to 3.355, 0; result = 70 | | | ✓ | |
| CmdZeroOutPeak | BL2000\mchavez | 1/10/2022 1:17:19 PM | Zero out primary peak of compound Methylene chloride in sample 05JAN14.D | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 1:17:31 PM | Set UserDefined = Qualifier ratio did not meet method criteria for Toluene for sample 05JAN14.D; previous value = | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 1:17:44 PM | Set UserDefined = Qualifier ratio did not meet method criteria for Methylene chloride for sample 05JAN14.D; previous value = Qualifier ratio did not meet method criteria for Toluene | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:18:15 PM | Manually integrate compound Benzene in sample 05JAN14.D from x, y = 6.238, 0 to 6.317, 0; result = 357 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:18:18 PM | Manually integrate qualifier77.0 of compound Benzene in sample 05JAN14.D from x, y = 6.269, 0 to 6.347, 0; result = 67 | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:18:34 PM | Manually integrate compound Bromodichloromethane in sample 05JAN14.D from x, y = 7.552, 0 to 7.624, 0; result = 1414 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:18:36 PM | Manually integrate qualifier85.0 of compound Bromodichloromethane in sample 05JAN14.D from x, y = 7.563, 0 to 7.630, 0; result = 808 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:18:39 PM | Manually integrate qualifier127.0 of compound Bromodichloromethane in sample 05JAN14.D from x, y = 7.558, 0 to 7.619, 0; result = 38 | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 1:18:43 PM | Set UserAnnotation = NI for compound Bromodichloromethane in sample 05JAN14.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 1:18:46 PM | Set UserAnnotation = NI for compound Benzene in sample 05JAN14.D; previous value = | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|--------------------------|----------------|----------------------|--|--------|---------|---------|--|
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:18:56 PM | Manually integrate compound Toluene in sample 05JAN14.D from x, y = 8.361, 0 to 8.408, 0; result = 0 | | | | Agilent.MassSpectrometry.DataAnalysis.Quantitative.ApplicationCommandException: Manual integration failed for compound Toluene in sample B22010002-001F. ---> Agilent.MassSpectrometry.DataAnalysis.Quantitative.ApplicationCommandException: Manual integration failed for compound Toluene in sample B22010002-001F. ---> System.IndexOutOfRangeException: Index was outside the bounds of the array. at Agilent.MassSpectrometry.DataAnalysis.AgileIntegrator.Peak.a(Double[] A_0, Single[] A_1, Int32 A_2, Int32 A_3, Int32 A_4, Double A_5, Double A_6, Double& A_7, Double& A_8, Int32& A_9, Int32& A_10, Int32& A_11, Int32& A_12) at Agilent.MassSpectrometry.DataAnalysis.AgileIntegrator.Peak.ComputeChromatographicMetrics(Double[] xArray, Single[] yArray, Int32 startIndex, Int32 apexIndex, Int32 endIndex, Double baselineSlope, Double yIntercept, Double& fullWidthHalfMaximum, Double& symmetry) at Agilent.MassSpectrometry.DataAnalysis.Quantitative.Integrator.a(IChromatogram A_0, IPeakList A_1) at Agilent.MassSpectrometry.DataAnalysis.Quantitative.Integrator.ManualIntegrate(IChromatogram chromatogram, Double xStart, Double yStart, Double xEnd, Double yEnd, IChromPeakList& peaklist) at Agilent.MassSpectrometry.DataAnalysis.Quantitative.Analysis.MeasuredIon.ManualIntegrate(Double xStart, Double yStart, Double xEnd, Double yEnd) --- End of inner exception stack trace --- at Agilent.MassSpectrometry.DataAnalysis.Quantitative.Analysis.QuantifierIon.SetManualIntegrationFailureMessage(Exception e) at Agilent.MassSpectrometry.DataAnalysis.Quantitative.Analysis.MeasuredIon.ManualIntegrate(Double xStart, Double yStart, Double xEnd, Double yEnd) |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|------|------|------|--------|--------|---------|---------|--|
| | | | | | | | at Agilent.MassSpectrometry.DataAnalysis.Quantitative.CmdManuallyIntegratePeak.Do() --- End of inner exception stack trace --- at Agilent.MassSpectrometry.DataAnalysis.Quantitative.CmdManuallyIntegratePeak.Do() at Agilent.MassSpectrometry.CommandModel.CommandHistory.Invoke(ICommand cmd) at Agilent.MassSpectrometry.DataAnalysis.Quantitative.AppCommandContext._Invoke(ICommand cmd) |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|---------------------------------------|----------------|----------------------|--|--------|---------|---------|--|
| CmdManuallyIntegrate QualifierPeak | BL2000\mchavez | 1/10/2022 1:19:03 PM | Manually integrate qualifier 91.0 of compound Toluene in sample 05JAN14.D from x, y = 8.363, 0 to 8.400, 0; result = 0 | | | | <p>Agilent.MassSpectrometry.DataAnalysis.Quantitative.ApplicationCommandException: Manual integration failed for qualifier 91.0 of compound Toluene in sample B22010002-001F. ---></p> <p>Agilent.MassSpectrometry.DataAnalysis.Quantitative.ApplicationCommandException: Manual integration failed for qualifier 91.0 of compound Toluene in sample B22010002-001F. ---></p> <p>System.IndexOutOfRangeException: Index was outside the bounds of the array.</p> <p>at at Agilent.MassSpectrometry.DataAnalysis.AgileIntegrator.Peak.a(Double[] A_0, Single[] A_1, Int32 A_2, Int32 A_3, Int32 A_4, Double A_5, Double A_6, Double& A_7, Double& A_8, Int32& A_9, Int32& A_10, Int32& A_11, Int32& A_12)</p> <p>at at Agilent.MassSpectrometry.DataAnalysis.AgileIntegrator.Peak.ComputeChromatographicMetrics(Double[] xArray, Single[] yArray, Int32 startIndex, Int32 apexIndex, Int32 endIndex, Double baselineSlope, Double yIntercept, Double& fullWidthHalfMaximum, Double& symmetry)</p> <p>at at Agilent.MassSpectrometry.DataAnalysis.Quantitative.Integrator.a(IChromatogram A_0, IPeakList A_1)</p> <p>at at Agilent.MassSpectrometry.DataAnalysis.Quantitative.Integrator.ManualIntegrate(IChromatogram chromatogram, Double xStart, Double yStart, Double xEnd, Double yEnd, IChromPeakList& peaklist)</p> <p>at at Agilent.MassSpectrometry.DataAnalysis.Quantitative.Analysis.MeasuredIon.ManualIntegrate(Double xStart, Double yStart, Double xEnd, Double yEnd)</p> <p>--- End of inner exception stack trace ---</p> <p>at at Agilent.MassSpectrometry.DataAnalysis.Quantitative.Analysis.QualifierIon.SetManualIntegrationFailureMessage(Exception e)</p> <p>at at Agilent.MassSpectrometry.DataAnalysis.Quantitative.Analysis.MeasuredIon.ManualIntegrate(Double xStart, Double yStart, Double xEnd, Double yEnd)</p> |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|---|--------|---------|---------|--|
| | | | | | | | at Agilent.MassSpectrometry.DataAnalysis.Quantitative.CmdManuallyIntegrateQualifierPeak.Do() --- End of inner exception stack trace --- at Agilent.MassSpectrometry.DataAnalysis.Quantitative.CmdManuallyIntegrateQualifierPeak.Do() at Agilent.MassSpectrometry.CommandModel.CommandHistory.Invoke(ICommand cmd) at Agilent.MassSpectrometry.DataAnalysis.Quantitative.AppCommandContext._Invoke(ICommand cmd) |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:19:09 PM | Manually integrate compound Toluene in sample 05JAN14.D from x, y = 8.358, 0 to 8.416, 0; result = 271 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:19:13 PM | Manually integrate qualifier91.0 of compound Toluene in sample 05JAN14.D from x, y = 8.358, 0 to 8.405, 0; result = 608 | | | ✓ | |
| CmdZeroOutPeak | BL2000\mchavez | 1/10/2022 1:19:18 PM | Zero out primary peak of compound Toluene in sample 05JAN14.D | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 1:19:31 PM | Set UserDefined = Qualifier ratio did not meet method criteria for Methylene chloride, Toluene for sample 05JAN14.D; previous value = Qualifier ratio did not meet method criteria for Methylene chloride | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:20:05 PM | Manually integrate compound Ethylbenzene in sample 05JAN14.D from x, y = 9.900, 0 to 9.939, 0; result = 333 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:20:07 PM | Manually integrate qualifier106.0 of compound Ethylbenzene in sample 05JAN14.D from x, y = 9.900, 0 to 9.939, 0; result = 56 | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 1:20:11 PM | Set UserAnnotation = NI for compound Ethylbenzene in sample 05JAN14.D; previous value = | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:20:16 PM | Manually integrate compound m+p-Xylenes in sample 05JAN14.D from x, y = 10.009, 0 to 10.090, 0; result = 479 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:20:19 PM | Manually integrate qualifier91.0 of compound m+p-Xylenes in sample 05JAN14.D from x, y = 9.995, 0 to 10.076, 0; result = 1538 | | | ✓ | |
| CmdZeroOutPeak | BL2000\mchavez | 1/10/2022 1:20:23 PM | Zero out primary peak of compound m+p-Xylenes in sample 05JAN14.D | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|---|--------|---------|---------|-----------|
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 1:20:45 PM | Set UserDefined = Qualifier ratio did not meet method criteria for Methylene chloride, Toluene, m+p Xylenes for sample 05JAN14.D; previous value = Qualifier ratio did not meet method criteria for Methylene chloride, Toluene | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 1:21:17 PM | Set SampleApproved = True for sample 05JAN14.D; previous value = False | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/10/2022 1:21:38 PM | Quantitate all compounds in all samples | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:22:11 PM | Manually integrate qualifier174.5 of compound Bromoform in sample 05JAN15.D from x, y = 10.580, 0 to 10.675, 0; result = 1921 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:22:13 PM | Manually integrate qualifier170.5 of compound Bromoform in sample 05JAN15.D from x, y = 10.580, 0 to 10.667, 0; result = 2415 | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:22:52 PM | Manually integrate compound Bromodichloromethane in sample 05JAN15.D from x, y = 7.541, 0 to 7.644, 0; result = 1705 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:22:55 PM | Manually integrate qualifier85.0 of compound Bromodichloromethane in sample 05JAN15.D from x, y = 7.541, 0 to 7.633, 0; result = 1225 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:22:57 PM | Manually integrate qualifier127.0 of compound Bromodichloromethane in sample 05JAN15.D from x, y = 7.566, 0 to 7.605, 0; result = 65 | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 1:23:01 PM | Set UserAnnotation = NI for compound Bromodichloromethane in sample 05JAN15.D; previous value = | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:24:09 PM | Manually integrate qualifier85.0 of compound Chloroform in sample 05JAN15.D from x, y = 5.586, 0 to 5.717, 0; result = 1954 | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:24:23 PM | Manually integrate compound Methylene chloride in sample 05JAN15.D from x, y = 3.296, 0 to 3.366, 0; result = 658 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:24:25 PM | Manually integrate qualifier84.0 of compound Methylene chloride in sample 05JAN15.D from x, y = 3.291, 0 to 3.372, 0; result = 283 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:24:27 PM | Manually integrate qualifier86.0 of compound Methylene chloride in sample 05JAN15.D from x, y = 3.293, 0 to 3.374, 0; result = 210 | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|---|--------|---------|---------|-----------|
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 1:24:39 PM | Set UserAnnotation = NI for compound Methylene chloride in sample 05JAN15.D; previous value = | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:24:55 PM | Manually integrate compound Chloromethane in sample 05JAN15.D from x, y = 1.386, 0 to 1.417, 0; result = 529 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:24:57 PM | Manually integrate qualifier 52.0 of compound Chloromethane in sample 05JAN15.D from x, y = 1.392, 0 to 1.453, 0; result = 111 | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 1:25:11 PM | Set UserAnnotation = NI for compound Chloromethane in sample 05JAN15.D; previous value = | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 1:25:14 PM | Set SampleApproved = True for sample 05JAN15.D; previous value = False | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:25:37 PM | Manually integrate qualifier 52.0 of compound Chloromethane in sample 05JAN16.D from x, y = 1.364, 0 to 1.464, 0; result = 1882 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:25:44 PM | Manually integrate qualifier 85.0 of compound Chloroform in sample 05JAN16.D from x, y = 5.603, 0 to 5.714, 0; result = 1868 | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:26:17 PM | Manually integrate compound Bromodichloromethane in sample 05JAN16.D from x, y = 7.541, 0 to 7.627, 0; result = 1814 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:26:18 PM | Manually integrate qualifier 85.0 of compound Bromodichloromethane in sample 05JAN16.D from x, y = 7.504, 0 to 7.532, 0; result = 0 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:26:20 PM | Manually integrate qualifier 85.0 of compound Bromodichloromethane in sample 05JAN16.D, from x, y = 7.504, 0 to 7.624, 0, result = 835; previous integration is from x, y = 7.504, 0 to 7.532, 0 and previous response = 0. | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:26:23 PM | Manually integrate qualifier 127.0 of compound Bromodichloromethane in sample 05JAN16.D from x, y = 7.557, 0 to 7.624, 0; result = 26 | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 1:26:27 PM | Set UserAnnotation = NI for compound Bromodichloromethane in sample 05JAN16.D; previous value = | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:26:34 PM | Manually integrate compound Benzene in sample 05JAN16.D from x, y = 6.238, 0 to 6.316, 0; result = 421 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:26:36 PM | Manually integrate qualifier 77.0 of compound Benzene in sample 05JAN16.D from x, y = 6.252, 0 to 6.297, 0; result = 28 | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|--|--------|---------|---------|-----------|
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 1:26:39 PM | Set UserAnnotation = NI for compound Benzene in sample 05JAN16.D; previous value = | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:26:48 PM | Manually integrate compound Toluene in sample 05JAN16.D from x, y = 8.358, 0 to 8.402, 0; result = 212 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:26:51 PM | Manually integrate qualifier91.0 of compound Toluene in sample 05JAN16.D from x, y = 8.361, 0 to 8.430, 0; result = 751 | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 1:26:56 PM | Set UserAnnotation = NI for compound Toluene in sample 05JAN16.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 1:27:01 PM | Set UserAnnotation = for compound Toluene in sample 05JAN16.D; previous value = NI | | | ✓ | |
| CmdZeroOutPeak | BL2000\mchavez | 1/10/2022 1:27:04 PM | Zero out primary peak of compound Toluene in sample 05JAN16.D | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:27:20 PM | Manually integrate compound m+p-Xylenes in sample 05JAN16.D from x, y = 10.011, 0 to 10.084, 0; result = 646 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:27:23 PM | Manually integrate qualifier91.0 of compound m+p-Xylenes in sample 05JAN16.D from x, y = 10.000, 0 to 10.073, 0; result = 1199 | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 1:27:27 PM | Set UserAnnotation = NI for compound m+p-Xylenes in sample 05JAN16.D; previous value = | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:27:34 PM | Manually integrate compound o-Xylene in sample 05JAN16.D from x, y = 10.388, 0 to 10.477, 0; result = 1444 | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 1:27:38 PM | Set UserAnnotation = NI for compound o-Xylene in sample 05JAN16.D; previous value = | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 1:27:59 PM | Set SampleApproved = True for sample 05JAN16.D; previous value = False | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/10/2022 1:28:17 PM | Quantitate all compounds in all samples | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:28:50 PM | Manually integrate compound m+p-Xylenes in sample 05JAN17.D from x, y = 10.017, 0 to 10.059, 0; result = 64 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:28:53 PM | Manually integrate qualifier91.0 of compound m+p-Xylenes in sample 05JAN17.D from x, y = 10.006, 0 to 10.076, 0; result = 130 | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 1:28:57 PM | Set UserAnnotation = NI for compound m+p-Xylenes in sample 05JAN17.D; previous value = | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|--|--------|---------|---------|-----------|
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:29:03 PM | Manually integrate compound Ethylbenzene in sample 05JAN17.D from x, y = 9.897, 0 to 9.939, 0; result = 97 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:29:05 PM | Manually integrate qualifier106.0 of compound Ethylbenzene in sample 05JAN17.D from x, y = 9.905, 0 to 9.939, 0; result = 64 | | | ✓ | |
| CmdZeroOutPeak | BL2000\mchavez | 1/10/2022 1:29:09 PM | Zero out primary peak of compound Ethylbenzene in sample 05JAN17.D | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 1:29:23 PM | Set UserDefined = Qualifier ratio did not meet method criteria for m+p Xylenes for sample 05JAN17.D; previous value = | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 1:29:34 PM | Set UserDefined = Qualifier ratio did not meet method criteria for Ethylbenzene for sample 05JAN17.D; previous value = Qualifier ratio did not meet method criteria for m+p Xylenes | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:30:16 PM | Manually integrate compound Methylene chloride in sample 05JAN17.D from x, y = 3.282, 0 to 3.377, 0; result = 599 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:30:18 PM | Manually integrate qualifier84.0 of compound Methylene chloride in sample 05JAN17.D from x, y = 3.294, 0 to 3.383, 0; result = 354 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:30:20 PM | Manually integrate qualifier86.0 of compound Methylene chloride in sample 05JAN17.D from x, y = 3.305, 0 to 3.361, 0; result = 53 | | | ✓ | |
| CmdZeroOutPeak | BL2000\mchavez | 1/10/2022 1:30:24 PM | Zero out primary peak of compound Methylene chloride in sample 05JAN17.D | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 1:30:40 PM | Set UserDefined = Qualifier ratio did not meet method criteria for Ethylbenzene, Methylene chloride for sample 05JAN17.D; previous value = Qualifier ratio did not meet method criteria for Ethylbenzene | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:30:54 PM | Manually integrate compound Methylene chloride in sample 05JAN16.D from x, y = 3.291, 0 to 3.383, 0; result = 894 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:30:56 PM | Manually integrate qualifier84.0 of compound Methylene chloride in sample 05JAN16.D from x, y = 3.294, 0 to 3.374, 0; result = 251 | | | ✓ | |
| CmdZeroOutPeak | BL2000\mchavez | 1/10/2022 1:31:00 PM | Zero out primary peak of compound Methylene chloride in sample 05JAN16.D | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|---|--------|---------|---------|-----------|
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 1:31:21 PM | Set UserDefined = Qualifier ratio did not meet method criteria for Methylene chloride for sample 05JAN16.D; previous value = | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:32:02 PM | Manually integrate compound Chloromethane in sample 05JAN17.D from x, y = 1.378, 0 to 1.442, 0; result = 1055 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:32:04 PM | Manually integrate qualifier52.0 of compound Chloromethane in sample 05JAN17.D from x, y = 1.392, 0 to 1.448, 0; result = 228 | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 1:32:11 PM | Set UserAnnotation = NI for compound Chloromethane in sample 05JAN17.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 1:32:12 PM | Set UserAnnotation = NI for compound Chloromethane in sample 05JAN17.D; previous value = NI | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 1:32:17 PM | Set SampleApproved = True for sample 05JAN17.D; previous value = False | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:32:36 PM | Manually integrate compound Methylene chloride in sample 05JAN18.D from x, y = 3.296, 0 to 3.388, 0; result = 441 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:32:38 PM | Manually integrate qualifier84.0 of compound Methylene chloride in sample 05JAN18.D from x, y = 3.305, 0 to 3.397, 0; result = 299 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:32:41 PM | Manually integrate qualifier86.0 of compound Methylene chloride in sample 05JAN18.D from x, y = 3.288, 0 to 3.386, 0; result = 175 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:33:14 PM | Manually integrate qualifier64.0 of compound 1,2-Dichloroethane in sample 05JAN18.D from x, y = 6.283, 0 to 6.361, 0; result = 1423 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:33:17 PM | Manually integrate qualifier98.0 of compound 1,2-Dichloroethane in sample 05JAN18.D from x, y = 6.291, 0 to 6.350, 0; result = 152 | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:34:08 PM | Manually integrate compound m+p-Xylenes in sample 05JAN18.D from x, y = 10.006, 0 to 10.070, 0; result = 54 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:34:11 PM | Manually integrate qualifier91.0 of compound m+p-Xylenes in sample 05JAN18.D from x, y = 10.011, 0 to 10.076, 0; result = 292 | | | ✓ | |
| CmdZeroOutPeak | BL2000\mchavez | 1/10/2022 1:34:15 PM | Zero out primary peak of compound m+p-Xylenes in sample 05JAN18.D | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|---|--------|---------|---------|-----------|
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 1:34:34 PM | Set UserDefined = Qualifier ratio did not meet method criteria for m+p Xylenes for sample 05JAN18.D; previous value = | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 1:35:00 PM | Set SampleApproved = True for sample 05JAN18.D; previous value = False | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/10/2022 1:35:20 PM | Quantitate all compounds in all samples | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/10/2022 1:37:48 PM | Quantitate all compounds in all samples | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:40:43 PM | Manually integrate compound Methylene chloride in sample 05JAN19.D from x, y = 3.305, 0 to 3.383, 0; result = 756 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:40:47 PM | Manually integrate qualifier 84.0 of compound Methylene chloride in sample 05JAN19.D from x, y = 3.296, 0 to 3.366, 0; result = 449 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:40:49 PM | Manually integrate qualifier 86.0 of compound Methylene chloride in sample 05JAN19.D from x, y = 3.296, 0 to 3.383, 0; result = 195 | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 1:40:54 PM | Set UserAnnotation = NI for compound Methylene chloride in sample 05JAN19.D; previous value = | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:41:11 PM | Manually integrate compound Chloromethane in sample 05JAN19.D from x, y = 1.383, 0 to 1.431, 0; result = 1360 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:41:14 PM | Manually integrate qualifier 52.0 of compound Chloromethane in sample 05JAN19.D from x, y = 1.367, 0 to 1.433, 0; result = 469 | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 1:41:18 PM | Set SampleApproved = True for sample 05JAN19.D; previous value = False | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 1:41:46 PM | Set UserAnnotation = NI for compound Chloromethane in sample 05JAN19.D; previous value = | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:44:21 PM | Manually integrate compound Benzene in sample 05JAN20.D from x, y = 6.261, 0 to 6.319, 0; result = 427 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:44:23 PM | Manually integrate qualifier 77.0 of compound Benzene in sample 05JAN20.D from x, y = 6.241, 0 to 6.291, 0; result = 68 | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:44:49 PM | Manually integrate compound m+p-Xylenes in sample 05JAN20.D from x, y = 10.025, 0 to 10.067, 0; result = 114 | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|---|--------|---------|---------|-----------|
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:44:51 PM | Manually integrate qualifier 91.0 of compound m+p-Xylenes in sample 05JAN20.D from x, y = 10.011, 0 to 10.056, 0; result = 129 | | | ✓ | |
| CmdZeroOutPeak | BL2000\mchavez | 1/10/2022 1:44:55 PM | Zero out primary peak of compound m+p-Xylenes in sample 05JAN20.D | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 1:45:07 PM | Set UserDefined = Qualifier ratio did not meet method criteria for m+p Xylenes for sample 05JAN20.D; previous value = | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 1:45:35 PM | Set SampleApproved = True for sample 05JAN20.D; previous value = False | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:46:18 PM | Manually integrate compound Benzene in sample 05JAN21.D from x, y = 6.238, 0 to 6.317, 0; result = 280 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:46:21 PM | Manually integrate qualifier 77.0 of compound Benzene in sample 05JAN21.D from x, y = 6.252, 0 to 6.319, 0; result = 25 | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:46:48 PM | Manually integrate compound Chloromethane in sample 05JAN21.D from x, y = 1.375, 0 to 1.445, 0; result = 1801 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:46:51 PM | Manually integrate qualifier 52.0 of compound Chloromethane in sample 05JAN21.D from x, y = 1.372, 0 to 1.462, 0; result = 449 | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 1:47:01 PM | Set UserAnnotation = NI for compound Chloromethane in sample 05JAN21.D; previous value = | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 1:47:03 PM | Set SampleApproved = True for sample 05JAN21.D; previous value = False | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 1:47:15 PM | Set UserAnnotation = NI for compound Benzene in sample 05JAN21.D; previous value = | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:47:44 PM | Manually integrate qualifier 52.0 of compound Chloromethane in sample 05JAN22.D from x, y = 1.364, 0 to 1.453, 0; result = 1415 | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:47:57 PM | Manually integrate compound Chloroethane in sample 05JAN22.D from x, y = 1.874, 224 to 1.913, 411; result = 1664 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:48:01 PM | Manually integrate qualifier 66.0 of compound Chloroethane in sample 05JAN22.D from x, y = 1.849, 0 to 1.913, 0; result = 417 | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 1:48:09 PM | Set UserAnnotation = NI for compound Chloroethane in sample 05JAN22.D; previous value = | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|--|--------|---------|---------|-----------|
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:48:16 PM | Manually integrate compound Methylene chloride in sample 05JAN22.D from x, y = 3.252, 662 to 3.313, 107; result = -1310 | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:48:19 PM | Manually integrate compound Methylene chloride in sample 05JAN22.D, from x, y = 3.282, 0 to 3.347, 21, result = 911; previous integration is from x, y = 3.252, 662 to 3.313, 107 and previous response = -1310. | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:48:22 PM | Manually integrate compound Methylene chloride in sample 05JAN22.D, from x, y = 3.282, 0 to 3.375, 0, result = 1094; previous integration is from x, y = 3.282, 0 to 3.347, 21 and previous response = 911. | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:48:24 PM | Manually integrate qualifier84.0 of compound Methylene chloride in sample 05JAN22.D from x, y = 3.296, 0 to 3.394, 0; result = 642 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:48:27 PM | Manually integrate qualifier86.0 of compound Methylene chloride in sample 05JAN22.D from x, y = 3.296, 0 to 3.372, 0; result = 335 | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:48:51 PM | Manually integrate compound Carbon tetrachloride in sample 05JAN22.D from x, y = 5.968, 0 to 6.077, 0; result = 1272 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:48:53 PM | Manually integrate qualifier119.0 of compound Carbon tetrachloride in sample 05JAN22.D from x, y = 5.965, 0 to 6.079, 0; result = 1217 | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:48:55 PM | Manually integrate qualifier121.0 of compound Carbon tetrachloride in sample 05JAN22.D from x, y = 5.993, 0 to 6.085, 0; result = 287 | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 1:49:00 PM | Set UserAnnotation = NI for compound Carbon tetrachloride in sample 05JAN22.D; previous value = | | | ✓ | |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:49:15 PM | Manually integrate compound Benzene in sample 05JAN22.D from x, y = 6.238, 0 to 6.333, 0; result = 1833 | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 1:49:17 PM | Set UserAnnotation = NI for compound Benzene in sample 05JAN22.D; previous value = | | | ✓ | |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:49:19 PM | Manually integrate qualifier77.0 of compound Benzene in sample 05JAN22.D from x, y = 6.236, 0 to 6.333, 0; result = 342 | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|--------------------------|----------------|----------------------|--|--------|---------|---------|-----------|
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:49:35 PM | Manually integrate compound 1,2-Dichloroethane in sample 05JAN22.D from x, y = 6.286, 0 to 6.375, 0; result = 1182 | | | ✓ | |
| CmdZeroOutPeak | BL2000\mchavez | 1/10/2022 1:49:38 PM | Zero out primary peak of compound 1,2-Dichloroethane in sample 05JAN22.D | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|--------------------------|----------------|----------------------|--|--------|---------|---------|--|
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:50:01 PM | Manually integrate compound Toluene in sample 05JAN22.D from x, y = 8.363, 0 to 8.408, 0; result = 0 | | | | Agilent.MassSpectrometry.DataAnalysis.Quantitative.ApplicationCommandException: Manual integration failed for compound Toluene in sample B22010143-001F. ---> Agilent.MassSpectrometry.DataAnalysis.Quantitative.ApplicationCommandException: Manual integration failed for compound Toluene in sample B22010143-001F. ---> System.IndexOutOfRangeException: Index was outside the bounds of the array. at Agilent.MassSpectrometry.DataAnalysis.AgileIntegrator.Peak.a(Double[] A_0, Single[] A_1, Int32 A_2, Int32 A_3, Int32 A_4, Double A_5, Double A_6, Double& A_7, Double& A_8, Int32& A_9, Int32& A_10, Int32& A_11, Int32& A_12) at Agilent.MassSpectrometry.DataAnalysis.AgileIntegrator.Peak.ComputeChromatographicMetrics(Double[] xArray, Single[] yArray, Int32 startIndex, Int32 apexIndex, Int32 endIndex, Double baselineSlope, Double yIntercept, Double& fullWidthHalfMaximum, Double& symmetry) at Agilent.MassSpectrometry.DataAnalysis.Quantitative.Integrator.a(IChromatogram A_0, IPeakList A_1) at Agilent.MassSpectrometry.DataAnalysis.Quantitative.Integrator.ManualIntegrate(IChromatogram chromatogram, Double xStart, Double yStart, Double xEnd, Double yEnd, IChromPeakList& peaklist) at Agilent.MassSpectrometry.DataAnalysis.Quantitative.Analysis.MeasuredIon.ManualIntegrate(Double xStart, Double yStart, Double xEnd, Double yEnd) --- End of inner exception stack trace --- at Agilent.MassSpectrometry.DataAnalysis.Quantitative.Analysis.QuantifierIon.SetManualIntegrationFailureMessage(Exception e) at Agilent.MassSpectrometry.DataAnalysis.Quantitative.Analysis.MeasuredIon.ManualIntegrate(Double xStart, Double yStart, Double xEnd, Double yEnd) |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|--|--------|---------|---------|--|
| | | | | | | | at Agilent.MassSpectrometry.DataAnalysis.Quantitative.CmdManuallyIntegratePeak.Do() --- End of inner exception stack trace --- at Agilent.MassSpectrometry.DataAnalysis.Quantitative.CmdManuallyIntegratePeak.Do() at Agilent.MassSpectrometry.CommandModel.CommandHistory.Invoke(ICommand cmd) at Agilent.MassSpectrometry.DataAnalysis.Quantitative.AppCommandContext._Invoke(ICommand cmd) |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:50:07 PM | Manually integrate qualifier 91.0 of compound Toluene in sample 05JAN22.D from x, y = 8.347, 0 to 8.402, 0; result = 0 | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|--------------------------|----------------|----------------------|--|--------|---------|---------|--|
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:50:10 PM | Manually integrate compound Toluene in sample 05JAN22.D from x, y = 8.361, 0 to 8.400, 0; result = 0 | | | | Agilent.MassSpectrometry.DataAnalysis.Quantitative.ApplicationCommandException: Manual integration failed for compound Toluene in sample B22010143-001F. ---> Agilent.MassSpectrometry.DataAnalysis.Quantitative.ApplicationCommandException: Manual integration failed for compound Toluene in sample B22010143-001F. ---> System.IndexOutOfRangeException: Index was outside the bounds of the array. at Agilent.MassSpectrometry.DataAnalysis.AgileIntegrator.Peak.a(Double[] A_0, Single[] A_1, Int32 A_2, Int32 A_3, Int32 A_4, Double A_5, Double A_6, Double& A_7, Double& A_8, Int32& A_9, Int32& A_10, Int32& A_11, Int32& A_12) at Agilent.MassSpectrometry.DataAnalysis.AgileIntegrator.Peak.ComputeChromatographicMetrics(Double[] xArray, Single[] yArray, Int32 startIndex, Int32 apexIndex, Int32 endIndex, Double baselineSlope, Double yIntercept, Double& fullWidthHalfMaximum, Double& symmetry) at Agilent.MassSpectrometry.DataAnalysis.Quantitative.Integrator.a(IChromatogram A_0, IPeakList A_1) at Agilent.MassSpectrometry.DataAnalysis.Quantitative.Integrator.ManualIntegrate(IChromatogram chromatogram, Double xStart, Double yStart, Double xEnd, Double yEnd, IChromPeakList& peaklist) at Agilent.MassSpectrometry.DataAnalysis.Quantitative.Analysis.MeasuredIon.ManualIntegrate(Double xStart, Double yStart, Double xEnd, Double yEnd) --- End of inner exception stack trace --- at Agilent.MassSpectrometry.DataAnalysis.Quantitative.Analysis.QuantifierIon.SetManualIntegrationFailureMessage(Exception e) at Agilent.MassSpectrometry.DataAnalysis.Quantitative.Analysis.MeasuredIon.ManualIntegrate(Double xStart, Double yStart, Double xEnd, Double yEnd) |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|--|--------|---------|---------|--|
| | | | | | | | at Agilent.MassSpectrometry.DataAnalysis.Quantitative.CmdManuallyIntegratePeak.Do() --- End of inner exception stack trace --- at Agilent.MassSpectrometry.DataAnalysis.Quantitative.CmdManuallyIntegratePeak.Do() at Agilent.MassSpectrometry.CommandModel.CommandHistory.Invoke(ICommand cmd) at Agilent.MassSpectrometry.DataAnalysis.Quantitative.AppCommandContext._Invoke(ICommand cmd) |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 1:50:15 PM | Manually integrate qualifier 91.0 of compound Toluene in sample 05JAN22.D from x, y = 8.347, 0 to 8.405, 0; result = 0 | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|--------------------------|----------------|----------------------|--|--------|---------|---------|---|
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:50:19 PM | Manually integrate compound Toluene in sample 05JAN22.D from x, y = 8.363, 0 to 8.402, 0; result = 0 | | | | <p>Agilent.MassSpectrometry.DataAnalysis.Quantitative.ApplicationCommandException: Manual integration failed for compound Toluene in sample B22010143-001F. ---></p> <p>Agilent.MassSpectrometry.DataAnalysis.Quantitative.ApplicationCommandException: Manual integration failed for compound Toluene in sample B22010143-001F. ---></p> <p>System.IndexOutOfRangeException: Index was outside the bounds of the array. at Agilent.MassSpectrometry.DataAnalysis.AgileIntegrator.Peak.a(Double[] A_0, Single[] A_1, Int32 A_2, Int32 A_3, Int32 A_4, Double A_5, Double A_6, Double& A_7, Double& A_8, Int32& A_9, Int32& A_10, Int32& A_11, Int32& A_12) at Agilent.MassSpectrometry.DataAnalysis.AgileIntegrator.Peak.ComputeChromatographicMetrics(Double[] xArray, Single[] yArray, Int32 startIndex, Int32 apexIndex, Int32 endIndex, Double baselineSlope, Double yIntercept, Double& fullWidthHalfMaximum, Double& symmetry) at Agilent.MassSpectrometry.DataAnalysis.Quantitative.Integrator.a(IChromatogram A_0, IPeakList A_1) at Agilent.MassSpectrometry.DataAnalysis.Quantitative.Integrator.ManualIntegrate(IChromatogram chromatogram, Double xStart, Double yStart, Double xEnd, Double yEnd, IChromPeakList& peaklist) at Agilent.MassSpectrometry.DataAnalysis.Quantitative.Analysis.MeasuredIon.ManualIntegrate(Double xStart, Double yStart, Double xEnd, Double yEnd) --- End of inner exception stack trace --- at Agilent.MassSpectrometry.DataAnalysis.Quantitative.Analysis.QuantifierIon.SetManualIntegrationFailureMessage(Exception e) at Agilent.MassSpectrometry.DataAnalysis.Quantitative.Analysis.MeasuredIon.ManualIntegrate(Double xStart, Double yStart, Double xEnd, Double yEnd)</p> |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-------------------------------|----------------|----------------------|--|--------|---------|---------|---|
| | | | | | | | at Agilent.MassSpectrometry.DataAnalysis.Quantitative.CmdManuallyIntegratePeak.Do() --- End of inner exception stack trace --- at Agilent.MassSpectrometry.DataAnalysis.Quantitative.CmdManuallyIntegratePeak.Do() at Agilent.MassSpectrometry.CommandModel.CommandHistory.Invoke(ICommand cmd) at Agilent.MassSpectrometry.DataAnalysis.Quantitative.AppCommandContext.Invoke(ICommand cmd) |
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/10/2022 1:50:28 PM | Manually integrate compound Toluene in sample 05JAN22.D from x, y = 8.375, 0 to 8.394, 0; result = 260 | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 1:50:33 PM | Set UserAnnotation = NI for compound Toluene in sample 05JAN22.D; previous value = | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 1:50:55 PM | Set SampleApproved = True for sample 05JAN22.D; previous value = False | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/10/2022 1:51:15 PM | Quantitate all compounds in all samples | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 1:55:55 PM | Set SampleApproved = True for sample 05JAN24.D; previous value = False | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 1:56:48 PM | Set SampleApproved = True for sample 05JAN25.D; previous value = False | | | ✓ | |
| CmdSetSampleAttribute | BL2000\mchavez | 1/10/2022 1:57:47 PM | Set SampleApproved = True for sample 05JAN27.D; previous value = False | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 1:58:38 PM | Set UserAnnotation = NI for compound Methylene chloride in sample 05JAN22.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/10/2022 2:01:18 PM | Set UserAnnotation = NI for compound Methylene chloride in sample 05JAN18.D; previous value = | | | ✓ | |
| CmdSaveBatchTable | BL2000\mchavez | 1/10/2022 2:13:09 PM | Save batch D:\Org\Data\VOA5975C\VG010522\QuantResults\VG010522_8260B.batch.bin | | | ✓ | |
| CmdOpenBatchTable | BL2000\mchavez | 1/11/2022 8:58:41 AM | Open batch D:\Org\Data\VOA5975C\VG010522\VG010522_8260B.batch.bin | | | ✓ | |
| CmdStartMethodEditing | BL2000\mchavez | 1/11/2022 8:58:58 AM | Start method editing | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-------------------------------|----------------|----------------------|---|--------|---------|---------|-----------|
| CmdImportMethodFromFile | BL2000\mchavez | 1/11/2022 8:58:59 AM | Import method from file \\MASSHUNTER\Org\Data\Methods\Quant\VOA5975C\VOA5975C_010422_CAL\VOA5975C_8260B_SHT_DoD_L4_010422.m | | | ✓ | |
| CmdApplyMethodToAllSamples | BL2000\mchavez | 1/11/2022 8:59:14 AM | Apply method to all samples | | | ✓ | |
| CmdMethodClear | BL2000\mchavez | 1/11/2022 8:59:14 AM | Clear method | | | ✓ | |
| CmdEndMethodEditing | BL2000\mchavez | 1/11/2022 8:59:15 AM | End method editing | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 1/11/2022 8:59:35 AM | Quantitate all compounds in all samples | | | ✓ | |
| CmdSaveBatchTable | BL2000\mchavez | 1/11/2022 9:07:57 AM | Save batch D:\Org\Data\VOA5975C\VG010522\QuantResults\VG010522_8260B.batch.bin | | | ✓ | |
| CmdOpenBatchTable | BL2000\mchavez | 2/28/2022 2:42:09 PM | Open batch D:\Org\Data\VOA5975C\VG010522\VG010522_8260B.batch.bin | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 2/28/2022 2:43:26 PM | Set UserAnnotation = NI for compound Chloromethane in sample 05JAN10.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 2/28/2022 2:43:48 PM | Set UserAnnotation = NI for compound Benzene in sample 05JAN12.D; previous value = | | | ✓ | |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 2/28/2022 2:45:09 PM | Set UserAnnotation = NI for compound Benzene in sample 05JAN20.D; previous value = | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|--------------|----------------|----------------------|---|--------|---------|---------|-----------|
| CmdCalibrate | BL2000\mchavez | 2/28/2022 2:46:37 PM | Replace level QC with QC sample 05JAN04.D for compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, o-Xylene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, 1,2-Dichloroethane, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1-Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Chloroethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, Benzene}; Replace level CC with CC sample 05JAN03.D for compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, o-Xylene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, 1,2-Dichloroethane, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1-Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-------------------|----------------|----------------------|---|--------|---------|---------|-----------|
| | | | ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Chloroethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, Benzene}; | | | | |
| CmdQuantitate | BL2000\mchavez | 2/28/2022 2:46:59 PM | Quantitate all compounds in all samples | | | ✓ | |
| CmdSaveBatchTable | BL2000\mchavez | 2/28/2022 2:47:19 PM | Save batch D:\Org\Data\VOA5975C\VG010522\QuantResults\VG010522_8260B.batch.bin | | | ✓ | |
| GenerateReport | BL2000\mchavez | 2/28/2022 2:48:22 PM | Generates report - Method: \\MASSHUNTER\Org\reports\LevelIV_Reports\SampleSequence\CC_mid_rpt.m, Output Path: D:\Org\Data\VOA5975C\VG010522\QuantReports\VG010522_8260B | | | ✓ | |
| CmdCalibrate | BL2000\mchavez | 2/28/2022 2:48:48 PM | Replace level CC with CC sample 05JAN27.D for compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, o-Xylene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, 1,2-Dichloroethane, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1-Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Chloroethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, Benzene}; | | | ✓ | |
| CmdQuantitate | BL2000\mchavez | 2/28/2022 2:49:11 PM | Quantitate all compounds in all samples | | | ✓ | |

Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception |
|-------------------|----------------|----------------------|---|--------|---------|---------|-----------|
| CmdSaveBatchTable | BL2000\mchavez | 2/28/2022 2:49:26 PM | Save batch D:\Org\Data\VOA5975C\VG010522\QuantResults\VG010522_8260B.batch.bin | | | ✓ | |
| GenerateReport | BL2000\mchavez | 2/28/2022 2:50:08 PM | Generates report - Method: \\MASSHUNTER\Org\reports\LevelIV_Reports\SampleSequence\CC_mid_rpt.m, Output Path: D:\Org\Data\VOA5975C\VG010522\QuantReports\VG010522_8260B-1 | | | ✓ | |



Analytical RunID VOA5975C.I_220104A Standards Traceability Report

Standard ID: VOCF0313

Standard Name: Liquids

Prep Date: 6/23/2020

Exp Date: 4/13/2023

Department: gcmsvoa

Vendor: AccuStd

Lot Number: 220041126

Balance ID:

Comments: Date Prepared is same as Date Received. 2,000 ug/mL. Catalog # M502A-R-10X. Corrected lot number to match Cl. MSC 01/14/2022

Type: Primary

Prep By: Alethea M. Shaules

Status: New

Final Volume: 10 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|--------------------------------------|--------------|-----|-------|-----------|
| Volatile Organic Compounds - Liquids | <u>12797</u> | 1 | mL | 4/13/2023 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0313 | ug/mL | |



Analytical RunID VOA5975C.I_220104A Standards Traceability Report

Spike ID: VOCF0352

Spike Name: 2nd Source Liquids

Prep Date: 11/23/2020

Exp Date: 12/31/2023

Department: gcmsvoa

Vendor: Agilent

Lot Number: 0006570990

Balance ID:

Comments: Date Prepared is same as Date Received. 2000 ug/mL in MeOH. Catalog # DWM-589N-1.

Type: Primary

Prep By: Steve Dilts

Status: New

Final Volume: 10 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|-----------------------|--------------|-----|-------|------------|
| VOC Standard | <u>13292</u> | 1 | mL | 12/31/2023 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0352 | ug/mL | |



Analytical RunID VOA5975C.I_220104A Standards Traceability Report

Spike ID: VOCF0364

Spike Name: Surrogates 2.0 mg/mL

Prep Date: 1/6/2021

Exp Date: 4/18/2029

Department: gcmsvoa

Vendor: AccuStandard

Lot Number: 219041458

Balance ID:

Comments: Date Received 01/04/2021. 2.0 mg/mL. Catalog # M-8260A-B-SS-10X

Type: Primary

Prep By: Jerran D. Brenden

Status: New

Final Volume: 10 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|------------------------|-----------|-----|-------|-----------|
| Surrogate Standard Mix | 13385 | 1 | mL | 4/18/2029 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0364 | ug/mL | |



Analytical RunID VOA5975C.I_220104A Standards Traceability Report

Standard ID: VOCF0373

Standard Name: MtBE (Methy tert-Butyl Ether)

Prep Date: 2/26/2021

Exp Date: 8/31/2022

Department: gcmsvoa

Vendor: Agilent

Lot Number: 0006555762

Balance ID:

Comments: Date Prepared is same as Date Received. 2000 ug/mL in MeOH. Catalog # STS-440

Type: Primary

Prep By: Steve Dilts

Status: New

Final Volume: 5 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|----------------------------------|-----------|-----|-------|-----------|
| Methyl tert-Butyl Ether Standard | 13578 | 1 | mL | 8/31/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0373 | ug/mL | |



Analytical RunID VOA5975C.I_220104A Standards Traceability Report

Spike ID: VOCF0401

Spike Name: 2nd Source MtBE

Prep Date: 6/7/2021

Exp Date: 12/11/2029

Department: gcmsvoa

Vendor: AccuStandard

Lot Number: 220051182

Balance ID:

Comments: Date Prepared is same as Date Receive. 2,000 ug/mL in MeOH. Catalog # S-078-10X.

Type: Primary

Prep By: Alethea M. Shaules

Status: New

Final Volume: 5 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|-----------------------|-----------|-----|-------|------------|
| MTBE | 13920 | 1 | mL | 12/11/2029 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0401 | ug/mL | |



Analytical RunID VOA5975C.I_220104A Standards Traceability Report

Spike ID: VOCF0417

Spike Name: Chem Service Gases

Type: Primary

Prep Date: 8/3/2021

Prep By: Steve Dilts

Exp Date: 2/28/2022

Status: New

Department: gcmsvoa

Vendor: Chemservice

Final Volume: 5 mL

Lot Number: 11882100

Balance ID:

Comments: Date Prepared is same as Date Received. 2000 ug/mL in MeOH. Catalog # M-VOHC6M5-1ML

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|---|--------------|-----|-------|-----------|
| Volatile Organics High Concentration Mixture #6 | <u>14142</u> | 5 | mL | 2/28/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0417 | ug/mL | |



Analytical RunID VOA5975C.I_220104A Standards Traceability Report

Standard ID: VOCF0425

Standard Name: Internals

Prep Date: 9/8/2021

Exp Date: 12/31/2022

Department: gcmsvoa

Vendor: Agilent

Lot Number: 0006582580

Balance ID:

Comments: Date Prepared is same as Date Received. 2,500 ug/mL in MeOH. Catalog # STM-520-1.

Type: Primary

Prep By: Jerran D. Brenden

Status: New

Final Volume: 10 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|-----------------------|--------------|-----|-------|------------|
| Internal Standard | <u>14251</u> | 1 | mL | 12/31/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0425 | ug/mL | |



Analytical RunID VOA5975C.I_220104A Standards Traceability Report

Spike ID: VOCF0426

Spike Name: Surrogates 2.0 mg/mL

Prep Date: 9/14/2021

Exp Date: 4/18/2029

Department: gcmsvoa

Vendor: AccuStandard

Lot Number: 219041458

Balance ID:

Comments: Date Received 01/04/2021. 2.0 mg/mL. Catalog # M-8260A-B-SS-10X

Type: Primary

Prep By: Jerran D. Brenden

Status: New

Final Volume: 10 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|------------------------|--------------|-----|-------|-----------|
| Surrogate Standard Mix | <u>14269</u> | 1 | mL | 4/18/2029 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0426 | ug/mL | |



Analytical RunID VOA5975C.I_220104A Standards Traceability Report

Standard ID: VOCF0427

Standard Name: Gases

Prep Date: 9/17/2021

Exp Date: 8/3/2024

Department: gcmsvoa

Vendor: Absolute

Lot Number: 080321

Balance ID:

Comments: Date Prepared is same as Date Received. 2,000 ug/mL in MeOH. Catalog # 30058.

Type: Primary

Prep By: Alethea M. Shaules

Status: New

Final Volume: 10 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|--|--------------|-----|-------|----------|
| EPA Method 502-524 - Volatile Gases Mix #1 | <u>14285</u> | 1 | mL | 8/3/2024 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0427 | ug/mL | |



Analytical RunID VOA5975C.I_220104A Standards Traceability Report

Standard ID: VOCF0434

Standard Name: Ketones

Prep Date: 10/26/2021

Exp Date: 6/30/2023

Department: gcmsvoa

Vendor: Chem Service

Lot Number: 10251200

Balance ID:

Comments: Date Prepared is same as Date Received. 2,000 ug/mL in 90:10 MeOH:H2O. Catalog # M-TCL-1AN5-5ML.

Type: Primary

Prep By: Steve Dilts

Status: New

Final Volume: 5 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|-----------------------|--------------|-----|-------|-----------|
| TCL Ketone Mix | <u>14443</u> | 1 | mL | 6/30/2023 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0434 | ug/mL | |



Analytical RunID VOA5975C.I_220104A Standards Traceability Report

Standard ID: VOCF0439

Standard Name: 2nd Source Ketones

Prep Date: 11/30/2021

Exp Date: 11/26/2022

Department: gcmsvoa

Vendor: AccuStandard

Lot Number: 221101480

Balance ID:

Comments: Date Prepared is same as Date Received. 2,000 ug/mL in Methanol. Catalog # CLP-022K-10X.

Type: Primary

Prep By: Melissa Chavez

Status: New

Final Volume: 1 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|-----------------------|--------------|-----|-------|------------|
| TCL Ketones Mixture | <u>14567</u> | 2 | mL | 11/26/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0439 | ug/mL | |



Analytical RunID VOA5975C.I_220104A Standards Traceability Report

Standard ID: VOFC3473

Standard Name: Calibration Surrogates

Prep Date: 9/14/2021

Exp Date: 3/14/2022

Department: gcmsvoa

Vendor:

Lot Number:

Balance ID:

Comments: Final Concentration 0.2 ug/uL in MeOH

Type: Secondary

Prep By: Jerran D. Brenden

Status: New

Final Volume: 5 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|--------------------------------|--------------|-----|-------|-----------|
| Methanol, Purge and Trap EA226 | <u>13754</u> | 4.5 | mL | 3/14/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0364 | ug/mL | 0.5 mL |



Analytical RunID VOA5975C.I_220104A Standards Traceability Report

Spike ID: VOCF3517

Spike Name: Internal Standard / Surrogates (INT/SURR)

Type: Secondary

Prep Date: 11/10/2021

Prep By: Alethea M. Shaules

Exp Date: 12/31/2022

Status: New

Department: gcmsvoa

Vendor:

Final Volume: 100 mL

Lot Number:

Balance ID:

Comments: Final Concentration 0.05 ug/uL in MeOH.

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|-------------------------------------|--------------|------|-------|------------|
| Methanol, Purge and Trap - EB199-US | <u>14334</u> | 95.5 | mL | 12/31/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0425 | ug/mL | 2 mL |
| VOCF0426 | ug/mL | 2.5 mL |



Analytical RunID VOA5975C.I_220104A Standards Traceability Report

Spike ID: VOCF3529B

Spike Name: 2nd Source MtBE

Prep Date: 11/29/2021

Exp Date: 1/29/2022

Department: gcmsvoa

Vendor:

Lot Number:

Balance ID:

Comments: Final Concentration 0.2 ug/uL

Type: Secondary

Prep By: Alethea M. Shaules

Status:

Final Volume: 10 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|-------------------------------------|--------------|-----|-------|-----------|
| Methanol, Purge and Trap - EB199-US | <u>14334</u> | 9 | mL | 1/29/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0401 | ug/mL | 1 mL |



Analytical RunID VOA5975C.I_220104A Standards Traceability Report

Standard ID: VOCF3546A

Standard Name: Liquids

Prep Date: 12/13/2021

Exp Date: 1/13/2022

Department: GCMSVOA

Vendor:

Lot Number:

Balance ID:

Comments: 1.0 ml/10 ml final volume. Final Concentration 0.2 ug/uL. Corrected comment and analyte list 11/9/2021 sbd

Type: Secondary

Prep By: Alethea M. Shaules

Status:

Final Volume: 10 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|--------------------------------|--------------|-----|-------|-----------|
| Methanol, Purge and Trap EA899 | <u>13926</u> | 9 | mL | 1/13/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0313 | ug/mL | 1 mL |



Analytical RunID VOA5975C.I_220104A Standards Traceability Report

Spike ID: VOCF3549

Spike Name: 2nd Source Ketones

Prep Date: 12/15/2021

Exp Date: 1/15/2022

Department: gcmsvoa

Vendor: AccuStandard

Lot Number: 221101480

Balance ID:

Comments: Vial opened for use. 2.0 µg/µL

Type: Primary

Prep By: Melissa Chavez

Status:

Final Volume: 1 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|-----------------------|--------------|-----|-------|-----------|
| TCL Ketones Mixture | <u>14567</u> | 1 | mL | 1/15/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0439 | ug/mL | 1 mL |



Analytical RunID VOA5975C.I_220104A Standards Traceability Report

Standard ID: VOFC3550

Standard Name: Ketones

Prep Date: 12/16/2021

Exp Date: 1/16/2022

Department: gcmsvoa

Vendor: Chem Service

Lot Number: 10251200

Balance ID:

Comments: Vial Opened For Use . 2.0 ug/uL in 90:10 MeOH:H2O.

Type: Primary

Prep By: Melissa Chavez

Status:

Final Volume: 1 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|-----------------------|--------------|-----|-------|-----------|
| TCL Ketone Mix | <u>14443</u> | 1 | mL | 1/16/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0434 | ug/mL | 1 mL |



Analytical RunID VOA5975C.I_220104A Standards Traceability Report

Spike ID: VOCF3558B

Spike Name: 2nd Source Liquids

Type: Secondary

Prep Date: 12/27/2021

Prep By: Steve Dilts

Exp Date: 2/27/2022

Status: Open

Department: gcmsvoa

Vendor:

Final Volume: 10 mL

Lot Number:

Balance ID:

Comments: Final Concentration 0.2ug/uL.

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|-------------------------------------|--------------|-----|-------|-----------|
| Methanol, Purge and Trap - EB199-US | <u>14334</u> | 9 | mL | 2/27/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0352 | ug/mL | 1 mL |



Analytical RunID VOA5975C.I_220104A Standards Traceability Report

Standard ID: VOCF3559A

Standard Name: MtBE

Prep Date: 12/27/2021

Exp Date: 1/27/2022

Department: gcmsvoa

Vendor:

Lot Number:

Balance ID:

Comments: Final Concentration 0.2 ug/uL.

Type: Secondary

Prep By: Melissa Chavez

Status:

Final Volume: 10 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|-------------------------------------|--------------|-----|-------|-----------|
| Methanol, Purge and Trap - EB199-US | <u>14334</u> | 9 | mL | 1/27/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0373 | ug/mL | 1 mL |



Analytical RunID VOA5975C.I_220104A Standards Traceability Report

Standard ID: VOCF3562A

Standard Name: Gases

Prep Date: 1/3/2022

Exp Date: 1/10/2022

Department: GCMSVOA

Vendor:

Lot Number:

Balance ID:

Comments: 1.0 ml/10 ml final volume. Final Concentration 0.2 ug/uL

Type: Secondary

Prep By: Alethea M. Shaules

Status:

Final Volume: 10 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|--------------------------------|--------------|-----|-------|-----------|
| Methanol, Purge and Trap EB373 | <u>14519</u> | 9 | mL | 1/10/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0427 | ug/mL | 1 mL |



Analytical RunID VOA5975C.I_220104A Standards Traceability Report

Standard ID: VOCF3563

Standard Name: Internals

Prep Date: 1/3/2022

Exp Date: 7/3/2022

Department: gcmsvoa

Vendor:

Lot Number:

Balance ID:

Comments: Final Concentration 0.05 ug/uL.

Type: Secondary

Prep By: Alethea M. Shaules

Status: New

Final Volume: 50 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|--------------------------------|--------------|-----|-------|----------|
| Methanol, Purge and Trap EB373 | <u>14519</u> | 49 | mL | 7/3/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0425 | ug/mL | 1 mL |



Analytical RunID VOA5975C.I_220104A Standards Traceability Report

Spike ID: VOFC3566A

Spike Name: 2nd Source Gases

Prep Date: 1/4/2022

Exp Date: 1/11/2022

Department: gcmsvoa

Vendor:

Lot Number:

Balance ID:

Comments: 1.0 ml/10 ml final volume. Final Concentration 0.2 ug/uL. Corrected final volume column to match comments and added final concentrations of analytes. MSC 01/14/2021

Type: Secondary

Prep By: Melissa Chavez

Status:

Final Volume: 10 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|--------------------------------|--------------|-----|-------|-----------|
| Methanol, Purge and Trap EB373 | <u>14519</u> | 9 | mL | 1/11/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0417 | ug/mL | 1 mL |

CERTIFICATE OF ANALYSIS

Catalog No: M-502A-R-10X
Description: Volatile Organic Compounds - Liquids
Lot: 220041126
Solvent: Methanol
Hazards: Refer to SDS for complete safety information

Date Certified: Apr 13, 2020
Expiration: Apr 13, 2023
Sample Size: 1 mL
Components: 54
Storage Condition: Refrig (0-5 °C)



Signal Word: Danger

Certified Reference Material



| Component | CAS # | Purity % (GC/MS) | Prepared Concentration* (µg/mL) | Certified Analyte Concentration* (µg/mL) |
|------------------------------|------------|---------------------|------------------------------------|---|
| Benzene | 71-43-2 | 100.0 | 2002 | 2002 |
| Bromobenzene | 108-86-1 | 100.0 | 2003 | 2003 |
| Bromochloromethane | 74-97-5 | 99.1 | 2001 | 1983 |
| Bromodichloromethane | 75-27-4 | 99.0 | 2002 | 1982 |
| Bromoform | 75-25-2 | 99.2 | 2001 | 1985 |
| n-Butylbenzene | 104-51-8 | 100.0 | 2002 | 2002 |
| sec-Butylbenzene | 135-98-8 | 100.0 | 2001 | 2001 |
| tert-Butylbenzene | 98-06-6 | 99.0 | 2003 | 1983 |
| Carbon tetrachloride | 56-23-5 | 100.0 | 2003 | 2003 |
| Chlorobenzene | 108-90-7 | 99.6 | 2001 | 1993 |
| Chloroform | 67-66-3 | 99.2 | 2004 | 1988 |
| 2-Chlorotoluene | 95-49-8 | 99.0 | 2003 | 1983 |
| 4-Chlorotoluene | 106-43-4 | 99.8 | 2002 | 1998 |
| Dibromochloromethane | 124-48-1 | 97.8 | 2049* | 2004 |
| 1,2-Dibromo-3-chloropropane | 96-12-8 | 99.2 | 2001 | 1985 |
| 1,2-Dibromoethane | 106-93-4 | 100.0 | 2006 | 2006 |
| Dibromomethane | 74-95-3 | 99.0 | 2002 | 1982 |
| 1,2-Dichlorobenzene | 95-50-1 | 98.2 | 2003 | 1967 |
| 1,3-Dichlorobenzene | 541-73-1 | 100.0 | 2000 | 2000 |
| 1,4-Dichlorobenzene | 106-46-7 | 100.0 | 2002 | 2002 |
| 1,1-Dichloroethane | 75-34-3 | 98.6 | 2001 | 1973 |
| 1,2-Dichloroethane | 107-06-2 | 99.8 | 2010 | 2006 |
| 1,1-Dichloroethene | 75-35-4 | 99.0 | 2000 | 1980 |
| cis-1,2-Dichloroethene | 156-59-2 | 99.0 | 2002 | 1982 |
| trans-1,2-Dichloroethene | 156-60-5 | 99.5 | 2001 | 1991 |
| 1,2-Dichloropropane | 78-87-5 | 99.5 | 2003 | 1993 |
| 1,3-Dichloropropane | 142-28-9 | 96.7 | 2073* | 2005 |
| 2,2-Dichloropropane | 594-20-7 | 99.9 | 2012 | 2010 |
| 1,1-Dichloropropene | 563-58-6 | 98.9 | 2001 | 1979 |
| cis-1,3-Dichloropropene ** | 10061-01-5 | 93.9 | 2041* | 1916 |
| trans-1,3-Dichloropropene ** | 10061-02-6 | 93.9 | 1968* | 1848 |
| Ethylbenzene | 100-41-4 | 99.7 | 2000 | 1994 |
| Hexachlorobutadiene | 87-68-3 | 98.0 | 2003 | 1963 |
| Isopropylbenzene | 98-82-8 | 100.0 | 2002 | 2002 |
| p-Isopropyltoluene | 99-87-6 | 99.4 | 2000 | 1988 |
| Methylene chloride | 75-09-2 | 99.9 | 2001 | 1999 |
| Naphthalene | 91-20-3 | 100.0 | 2002 | 2002 |
| n-Propylbenzene | 103-65-1 | 100.0 | 2001 | 2001 |
| Styrene | 100-42-5 | 100.0 | 2003 | 2003 |
| 1,1,1,2-Tetrachloroethane | 630-20-6 | 98.9 | 2005 | 1983 |
| 1,1,1,2,2-Tetrachloroethane | 79-34-5 | 96.0 | 2087* | 2004 |
| Tetrachloroethene | 127-18-4 | 99.4 | 2017 | 2005 |
| Toluene | 108-88-3 | 100.0 | 2001 | 2001 |
| 1,2,3-Trichlorobenzene | 87-61-6 | 100.0 | 2002 | 2002 |



CERTIFICATE OF ANALYSIS

Catalog No: M-502A-R-10X
Description: Volatile Organic Compounds - Liquids
Lot: 220041126
Solvent: Methanol

Date Certified: Apr 13, 2020
Expiration: Apr 13, 2023
Sample Size: 1 mL
Components: 54

| Component - <i>continued</i> | CAS # | Purity % | Prepared Concentration ² | Certified Analyte Concentration ¹ |
|------------------------------|----------|----------|-------------------------------------|--|
| | | (GC/MS) | (µg/mL) | (µg/mL) |
| 1,2,4-Trichlorobenzene | 120-82-1 | 99.6 | 2001 | 1993 |
| 1,1,1-Trichloroethane | 71-55-6 | 100.0 | 2002 | 2002 |
| 1,1,2-Trichloroethane | 79-00-5 | 98.6 | 2000 | 1972 |
| Trichloroethene | 79-01-6 | 100.0 | 2003 | 2003 |
| 1,2,3-Trichloropropane | 96-18-4 | 97.5 | 2055* | 2004 |
| 1,2,4-Trimethylbenzene | 95-63-6 | 98.2 | 2001 | 1965 |
| 1,3,5-Trimethylbenzene | 108-67-8 | 98.8 | 2001 | 1977 |
| o-Xylene | 95-47-6 | 99.0 | 2000 | 1980 |
| m-Xylene | 108-38-3 | 99.2 | 2002 | 1986 |
| p-Xylene | 106-42-3 | 95.4 | 2097* | 2001 |

* Weight compensated to 100% purity.

** 47.8% cis isomer, 46.1% trans isomer

A product with a suffix (-1A, -2B, etc. or -01, -02, etc.) on its lot number has had its expiration date extended and is identical to the same lot number without the suffix.

² All weights are traceable through NIST, Test No. 684/289871-17

¹ Certified Analyte Concentration = Purity x Prepared Concentration.

The Uncertainty associated with the certified concentration reported on this certificate is $\pm 2.4\%$. This value is the combined expanded uncertainty and represents an estimated standard deviation equal to the positive square root of the total variation of the uncertainty of components. A normal distribution is assumed and a coverage factor of K=2 is chosen using approximately a 95% confidence level.

Labels and certificates follow U.S. Conventions in reporting numerical values: A comma (,) is used to separate units of one-thousand or greater. A period (.) is used as a decimal place marker.

The information on this certificate may not be reproduced without the express permission of the manufacturer. See reverse side for additional information

Certified By:

Larry Decker, Organic QC Manager

ID #: 12797

Opened: _____

Volatile Organic Compounds - Liquids

Expires: 4/13/2023

Rec'd: 6/23/2020

Energy Laboratories Inc 1120 So. 27th Street
Billings MT 59107

Certificate of Analysis

Product Name: VOC Standard

Product Number: DWM-589N-1

Lot Number: 0006570990

Lot Issue Date: 17-Nov-2020

Expiration Date: 31-Dec-2023


Description:

This analytical reference material (RM) was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed below.

| Analyte | CAS# | Analyte Lot | Concentration ± Uncertainty |
|---------------------------|-------------|-------------|-----------------------------|
| bromochloromethane | 000074-97-5 | RM00009 | 2010 ± 10 µg/mL |
| bromodichloromethane | 000075-27-4 | RM12585 | 2009 ± 10 µg/mL |
| bromoform | 000075-25-2 | RM13987 | 2010 ± 10 µg/mL |
| carbon tetrachloride | 000056-23-5 | RM07576 | 2010 ± 10 µg/mL |
| chloroform | 000067-66-3 | RM13988 | 2009 ± 10 µg/mL |
| dibromochloromethane | 000124-48-1 | RM14843 | 2009 ± 10 µg/mL |
| dibromomethane | 000074-95-3 | RM12878 | 2009 ± 10 µg/mL |
| methylene chloride | 000075-09-2 | RM11650 | 2009 ± 10 µg/mL |
| 1,2-dibromoethane | 000106-93-4 | RM00018 | 2010 ± 10 µg/mL |
| 1,1-dichloroethane | 000075-34-3 | RM16217 | 2006 ± 10 µg/mL |
| 1,2-dichloroethane | 000107-06-2 | RM04655 | 2005 ± 10 µg/mL |
| 1,1-dichloroethene | 000075-35-4 | RM14486 | 2010 ± 10 µg/mL |
| cis-1,2-dichloroethene | 000156-59-2 | RM15008 | 2007 ± 10 µg/mL |
| trans-1,2-dichloroethene | 000156-60-5 | RM07565 | 2008 ± 10 µg/mL |
| 1,1,1,2-tetrachloroethane | 000630-20-6 | RM12632 | 2005 ± 10 µg/mL |
| 1,1,2,2-tetrachloroethane | 000079-34-5 | RM02540 | 2009 ± 10 µg/mL |
| tetrachloroethene | 000127-18-4 | RM06491 | 2008 ± 10 µg/mL |

Certificate of Analysis

| | | | |
|-----------------------------|-------------|--------------------|-----------------|
| Product Number: | DWM-589N-1 | Lot Number: | 0006570990 |
| 1,1,1-trichloroethane | 000071-55-6 | RM16539 | 2004 ± 10 µg/mL |
| 1,1,2-trichloroethane | 000079-00-5 | RM01175 | 2009 ± 10 µg/mL |
| trichloroethene | 000079-01-6 | RM14232 | 2009 ± 10 µg/mL |
| 1,2-dibromo-3-chloropropane | 000096-12-8 | RM13666 | 2009 ± 10 µg/mL |
| 1,2-dichloropropane | 000078-87-5 | RM12821 | 2008 ± 10 µg/mL |
| 1,3-dichloropropane | 000142-28-9 | RM02080 | 2008 ± 10 µg/mL |
| 2,2-dichloropropane | 000594-20-7 | RM12927 | 2005 ± 10 µg/mL |
| 1,1-dichloropropene | 000563-58-6 | RM16190 | 2010 ± 10 µg/mL |
| cis-1,3-dichloropropene | 010061-01-5 | RM12891 | 2007 ± 10 µg/mL |
| trans-1,3-dichloropropene | 010061-02-6 | RM12254 | 2006 ± 10 µg/mL |
| hexachlorobutadiene | 000087-68-3 | RM09157 | 2005 ± 10 µg/mL |
| 1,2,3-trichloropropane | 000096-18-4 | RM13082 | 2004 ± 10 µg/mL |
| benzene | 000071-43-2 | RM12931 | 2009 ± 10 µg/mL |
| n-butylbenzene | 000104-51-8 | RM03651 | 2008 ± 10 µg/mL |
| sec-butylbenzene | 000135-98-8 | RM10905 | 2005 ± 10 µg/mL |
| tert-butylbenzene | 000098-06-6 | RM14040 | 2007 ± 10 µg/mL |
| ethylbenzene | 000100-41-4 | RM12195 | 2006 ± 10 µg/mL |
| isopropylbenzene | 000098-82-8 | RM00835 | 2009 ± 10 µg/mL |
| 4-isopropyltoluene | 000099-87-6 | RM09747 | 2009 ± 10 µg/mL |
| naphthalene | 000091-20-3 | NT00970 | 2006 ± 10 µg/mL |
| n-propylbenzene | 000103-65-1 | RM12785 | 2010 ± 10 µg/mL |
| styrene | 000100-42-5 | RM13393 | 2010 ± 10 µg/mL |



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality Management System. Cert # 56 100 18560026

Page: 2 of 4

www.agilent.com/quality/
CSD-QA-015.1



ISO 17025 Cert
No. AT-1937



Certificate of Analysis

Product Number: DWM-589N-1

Lot Number: 0006570990

| | | | |
|------------------------|-------------|---------|-----------------|
| toluene | 000108-88-3 | RM06650 | 2008 ± 10 µg/mL |
| 1,2,4-trimethylbenzene | 000095-63-6 | RM06731 | 2002 ± 10 µg/mL |
| 1,3,5-trimethylbenzene | 000108-67-8 | RM12905 | 2009 ± 10 µg/mL |
| o-xylene | 000095-47-6 | RM15639 | 2005 ± 10 µg/mL |
| m-xylene | 000108-38-3 | RM15919 | 2006 ± 10 µg/mL |
| p-xylene | 000106-42-3 | RM02647 | 2009 ± 10 µg/mL |
| bromobenzene | 000108-86-1 | RM10227 | 2008 ± 10 µg/mL |
| chlorobenzene | 000108-90-7 | RM01874 | 2008 ± 10 µg/mL |
| 2-chlorotoluene | 000095-49-8 | RM13774 | 2007 ± 10 µg/mL |
| 4-chlorotoluene | 000106-43-4 | RM11750 | 2009 ± 10 µg/mL |
| 1,2-dichlorobenzene | 000095-50-1 | RM13636 | 2005 ± 10 µg/mL |
| 1,3-dichlorobenzene | 000541-73-1 | NT00356 | 2009 ± 10 µg/mL |
| 1,4-dichlorobenzene | 000106-46-7 | RM12826 | 2009 ± 10 µg/mL |
| 1,2,3-trichlorobenzene | 000087-61-6 | RM10193 | 2007 ± 10 µg/mL |
| 1,2,4-trichlorobenzene | 000120-82-1 | RM09454 | 2009 ± 10 µg/mL |

Matrix: methanol (methyl alcohol)

Storage Conditions: Store Frozen (-25° to -10°C).

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCCL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This RM was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality Management System. Cert # 56 100 18560026

Page: 3 of 4

www.agilent.com/quality/
CSD-QA-015.1



ISO 17025 Cert
No. AT-1937

Certificate of Analysis

Product Number: DWM-589N-1

Lot Number: 0006570990

Intended Use:

This RM is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Hazards:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this RM.

Expiration of Certification:

The certification of this RM is valid until the expiration date specified above, provided the RM is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the RM is damaged, contaminated, or otherwise modified.

Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:



Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality Management System. Cert # 56 100 18560026

Page: 4 of 4

www.agilent.com/quality/
CSD-QA-015.1



ISO 17025 Cert
No. AT-1937

Jewar

CERTIFICATE OF ANALYSIS

Catalog No: M-8260A-B-SS-10X
Description: Surrogate Standard Mix
Lot: 219041458

Solvent: Methanol
Hazards: Refer to SDS for complete safety information

Date Certified: Apr 18, 2019
Expiration: Apr 18, 2029
Sample Size: 1 mL
Components: 4
Storage Condition: Ambient (>5 °C)



Signal Word: Danger

Certified Reference Material



| Component | CAS # | Purity % (GC/MS) | Prepared Concentration ² (µg/mL) | Certified Analyte Concentration ¹ (µg/mL) |
|-----------------------|------------|---------------------|---|--|
| p-Bromofluorobenzene | 460-00-4 | 99.9 | 2004 | 2002 |
| Dibromofluoromethane | 1868-53-7 | 99.8 | 2005 | 2001 |
| 1,2-Dichloroethane-d4 | 17060-07-0 | 100.0 | 2001 | 2001 |
| Toluene-d8 | 2037-26-5 | 100.0 | 2000 | 2000 |

ID #: 13385
Opened: _____
Surrogate Standard Mix
Expires: 4/18/2029
Rec'd: 1/4/2021
Energy Laboratories Inc 1120 So. 27th Street
Billings MT 59107

A product with a suffix (-1A, -2B, etc. or -01, -02, etc.) on its lot number has had its expiration date extended and is identical to the same lot number without the suffix.

² All weights are traceable through NIST, Test No. 684/289871-17

¹ Certified Analyte Concentration = Purity x Prepared Concentration.


The Uncertainty associated with the certified concentration reported on this certificate is ±2.4%. This value is the combined expanded uncertainty and represents an estimated standard deviation equal to the positive square root of the total variation of the uncertainty of components. A normal distribution is assumed and a coverage factor of K=2 is chosen using approximately a 95% confidence level.

Labels and certificates follow U.S. Conventions in reporting numerical values: A comma (,) is used to separate units of one-thousand or greater. A period (.) is used as a decimal place marker.

The information on this certificate may not be reproduced without the express permission of the manufacturer. See reverse side for additional information

Hazard Information: Please refer to the SDS for information regarding the hazards associated with using this material.

This product was prepared according to in-house procedures and is guaranteed to be homogeneous.

Certified By: 
Larry Decker, Organic QC Manager

Certificate of Analysis

Product Name: Methyl tert-Butyl Ether Standard**Product Number:** STS-440-1**Lot Number:** 0006555762**Lot Issue Date:** 19-Aug-2020**Expiration Date:** 31-Aug-2022**Description:**

This analytical reference material (RM) was manufactured and verified in accordance with an ISO 9001 registered quality system, and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed below.

Analyte**CAS#****Analyte Lot****Concentration ± Uncertainty**

tert-butylmethyl ether

001634-04-4

RM06568

2006 ± 10 µg/mL

Matrix: methanol (methyl alcohol)**Storage Conditions:** Store Frozen (-25° to -10°C).**Traceability:**

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCCL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This RM was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Intended Use:

This RM is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Hazards:


Refer to the Safety Data Sheet on www.agilent.com for information regarding this RM.

Expiration of Certification:

The certification of this RM is valid until the expiration date specified above, provided the RM is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the RM is damaged, contaminated, or otherwise modified.

Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:

Monica Bourgeois

QMS Representative

ISO 17034 Cert
No. AR-1936RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality
Management System. Cert # 56 100 18560026

Page: 1 of 1

www.agilent.com/quality/
CSD-QA-015.1ISO 17025 Cert
No. AT-1937

CERTIFICATE OF ANALYSIS

Catalog No: S-078-10X

Description: MtBE

Lot: 220051182

Solvent: Methanol

Hazards: Refer to SDS for complete safety information

Date Certified: May 18, 2020

Expiration: May 18, 2030

Sample Size: 1 mL

Components: 1

Storage Condition: Ambient (>5 °C)



Signal Word: Danger

Certified Reference Material



| Component | CAS # | Purity % (GC/MS) | Prepared Concentration ² (µg/mL) | Certified Analyte Concentration ¹ (µg/mL) |
|-----------|-----------|---------------------|--|---|
| MtBE | 1634-04-4 | 100.0 | 2002 | 2002 |

ID #: 13920

Opened: _____

MTBE

Expires: 5/18/2030

Rec'd: 6/7/2021

Eneray Laboratories Inc 1120 So. 27th Street
Billings MT 59107

A product with a suffix (-1A, -2B, etc. or -01, -02, etc.) on its lot number has had its expiration date extended and is identical to the same lot number without the suffix.

² All weights are traceable through NIST, Test No. 684/289871-17

¹ Certified Analyte Concentration = Purity x Prepared Concentration.

The Uncertainty associated with the certified concentration reported on this certificate is $\pm 2.4\%$. This value is the combined expanded uncertainty and represents an estimated standard deviation equal to the positive square root of the total variation of the uncertainty of components. A normal distribution is assumed and a coverage factor of K=2 is chosen using approximately a 95% confidence level.

Labels and certificates follow U.S. Conventions in reporting numerical values: A comma (,) is used to separate units of one-thousand or greater. A period (.) is used as a decimal place marker.

The information on this certificate may not be reproduced without the express permission of the manufacturer. See reverse side for additional information

Hazard Information: Please refer to the SDS for information regarding the hazards associated with using this material.

This product was prepared according to in-house procedures and is guaranteed to be homogeneous.

Certified By: _____

Larry Decker, Organic QC Manager

CERTIFICATE OF ANALYSIS

CONCENTRATION 2000ug/ml in Methanol
CATALOG NUMBER M-VOHC6M5-1ML
LOT NUMBER 11882100
DATE CERTIFIED 05/25/21
EXPIRATION DATE 02/28/22
STORAGE Store at room temperature (20 - 25 °C).
HANDLING See Safety Data Sheet
INTENDED USE For laboratory use only.
ISO 17034:2016 CERTIFIED []

Volatile Organics High Concentration Mixture #6

ID #: 14142

Opened: _____

Volatile Organics High Concentration Mixture

Expires: 2/28/2022

Rec'd: 8/3/2021

Energx Laboratories Inc 1120 So. 27th Street
Billings MT 59107

| ID | Analyte | CAS | Weight Analyte (mg) | Lot | Purity | Certified Concentration (ug/mL) |
|---------|-------------------------|---------|---------------------|----------|--------|---------------------------------|
| N-11446 | Chloroethane | 75-00-3 | 96.300 | 00001728 | 100.0 | 2006.3 |
| N-11665 | Dichlorodifluoromethane | 75-71-8 | 96.610 | 00001729 | 100.0 | 2012.7 |
| N-12417 | Methyl bromide | 74-83-9 | 96.910 | 00024694 | 100.0 | 2019.0 |
| N-12421 | Methyl chloride | 74-87-3 | 96.150 | 00001731 | 100.0 | 2003.1 |
| N-13655 | Trichlorofluoromethane | 75-69-4 | 96.300 | 00027239 | 99.4 | 1994.2 |
| N-13748 | Vinyl chloride | 75-01-4 | 96.150 | 00019298 | 100.0 | 2003.1 |

Analytical Test

Value

CONCENTRATION (GC/MSD)

VERIFIED

CHEM SERVICE INC

660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599
1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729
info@chemservice.com • www.chemservice.com

Instructions for Use:

Shake mixture prior to use. If particles are present, sonicate for homogeneity. If sample is diluted to lower concentrations, Class A volumetric glassware must be used.

Minimum Sample Size- 0.2 uL for Direct Injection.

Chem Service Inc. guarantees the expanded uncertainty of the above analytes to be +/- 2.0% of the certified concentrations based on gravimetric preparation. The test results published in this report were obtained using equipment capable of producing results that are traceable to NIST and through NIST to the International System of Units (SI). The reported expanded uncertainty of measurement is stated as the combined standard uncertainty of measurement multiplied by the coverage factor k (k=2) such that the coverage probability corresponds to approximately 95%. For certified reference materials, homogeneity and thermal stability testing are available upon request.

Certified By:

Mary Beth O'Donnell

Mary Beth O'Donnell
CSM/TC





660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599
1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729
info@chemservice.com • www.chemservice.com

CERTIFICATE OF ANALYSIS

Analysis Method:

Catalog Number: M-VOHC6M5-1ML
Description: Volatile Organics High Concentration Mixture #6
Lot Number: 11882100
Expiration Date: 02/28/22

Abundance





Certificate of Analysis

ID #: 14251

Opened: _____

Internal Standard

Expires: 12/31/2022

Rec'd: 9/8/2021

Energy Laboratories Inc 1120 So. 27th Street
Billings MT 59107

Product Name: Internal Standard

Product Number: STM-520-1

Lot Issue Date: 05-Jan-2021

Lot Number: 0006582580

Expiration Date: 31-Dec-2022

Description:

This analytical reference material (RM) was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed below.

| Analyte | CAS# | Analyte Lot | Concentration ± Uncertainty |
|------------------------|-------------|-------------|-----------------------------|
| chlorobenzene-d5 | 003114-55-4 | RM12274 | 2501 ± 13 µg/mL |
| 1,4-dichlorobenzene-d4 | 003855-82-1 | RM12517 | 2501 ± 13 µg/mL |
| fluorobenzene | 000462-06-6 | RM13378 | 2512 ± 13 µg/mL |

Matrix: methanol (methyl alcohol)

Storage Conditions: Store Frozen (-25° to -10°C).

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCCL Z540.3, ISO 9001, ISO 17025 and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This RM was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Intended Use:

This RM is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Hazards:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this RM.



ISO 17034
REFERENCE MATERIAL
PRODUCER
ISO 17034 Cert
No. AR-1936

RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality Management System. Cert # 56 100 18560026

Page: 1 of 2

www.agilent.com/quality/
CSD-QA-015.1



ISO 17025 Cert
No. AT-1937



Certificate of Analysis

Product Number: STM-520-1

Lot Number: 0006582580

Expiration of Certification:

The certification of this RM is valid until the expiration date specified above, provided the RM is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the RM is damaged, contaminated, or otherwise modified.

Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:

Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality Management System. Cert # 56 100 18560026

Page: 2 of 2

www.agilent.com/quality/
CSD-QA-015.1



ISO 17025 Cert
No. AT-1937

CERTIFICATE OF ANALYSIS

Catalog No: M-8260A-B-SS-10X
Description: Surrogate Standard Mix
Lot: 219041458

Solvent: Methanol

Hazards: Refer to SDS for complete safety information

Date Certified: Apr 18, 2019

Expiration: Apr 18, 2029

Sample Size: 1 mL

Components: 4

Storage Condition: Ambient (>5 °C)



Signal Word: Danger

Certified Reference Material



| Component | CAS # | Purity % (GC/MS) | Prepared Concentration ² (µg/mL) | Certified Analyte Concentration ¹ (µg/mL) |
|-----------------------|------------|---------------------|---|--|
| p-Bromofluorobenzene | 460-00-4 | 99.9 | 2004 | 2002 |
| Dibromofluoromethane | 1868-53-7 | 99.8 | 2005 | 2001 |
| 1,2-Dichloroethane-d4 | 17060-07-0 | 100.0 | 2001 | 2001 |
| Toluene-d8 | 2037-26-5 | 100.0 | 2000 | 2000 |

ID #: 14269

Opened: _____

Surrogate Standard Mix

Expires: 4/18/2029

Rec'd: 9/14/2021

Energy Laboratories Inc 1120 So. 27th Street
Billings MT 59107

A product with a suffix (-1A, -2B, etc. or -01, -02, etc.) on its lot number has had its expiration date extended and is identical to the same lot number without the suffix.

² All weights are traceable through NIST, Test No. 684/289871-17

¹ Certified Analyte Concentration = Purity x Prepared Concentration.

The Uncertainty associated with the certified concentration reported on this certificate is $\pm 2.4\%$. This value is the combined expanded uncertainty and represents an estimated standard deviation equal to the positive square root of the total variation of the uncertainty of components. A normal distribution is assumed and a coverage factor of K=2 is chosen using approximately a 95% confidence level.

Labels and certificates follow U.S. Conventions in reporting numerical values: A comma (,) is used to separate units of one-thousand or greater. A period (.) is used as a decimal place marker.



The information on this certificate may not be reproduced without the express permission of the manufacturer. See reverse side for additional information

Hazard Information: Please refer to the SDS for information regarding the hazards associated with using this material.

This product was prepared according to in-house procedures and is guaranteed to be homogeneous.

Certified By: _____

Larry Decker, Organic QC Manager



CERTIFIED WEIGHT REPORT

Part Number: 30058
Lot Number: 080321
Description: EPA Method 502/524 - Volatile Gases Mix #1
6 components
Expiration Date: 080324
Recommended Storage: Freezer (0 °C)
Nominal Concentration (µg/mL): 2000
NIST Test ID#: 6UTB
Solvent: Methanol
Lot#: EA783-US
5E-05 Balance Uncertainty
Weight(s) shown below were combined and diluted to (mL): 500.0 0.058 Flask Uncertainty


| | | |
|----------------|-----------------|--------|
| Formulated By: | Mario Luis | 080321 |
| | | DATE |
| Reviewed By: | Pedro L. Rentas | 080321 |
| | | DATE |

| Compound | RM# | Lot Number | Nominal Conc (µg/mL) | Purity (%) | Uncertainty Purity (%) | Target Weight (g) | Actual Weight (g) | Actual Conc(µg/mL) | Expanded Uncertainty (+/-) (µg/mL) | SDS Information (Solvent Safety Info. On Attached pg.) | | |
|----------------------------|-----|------------|----------------------|------------|------------------------|-------------------|-------------------|--------------------|------------------------------------|--|---------------------------|-------------------|
| | | | | | | | | | | CAS# | OSHA PEL (TWA) | LD50 |
| 1. Bromomethane | 50 | 01611JX | 2000 | 99.5 | 0.2 | 1.00508 | 1.0098 | 2009.4 | 8.1 | 74-83-9 | 5 ppm (20mg/m3/8H) (skin) | ori-rat 214mg/kg |
| 2. Chloroethane | 72 | 062617 | 2000 | 99 | 0.2 | 1.01016 | 1.0146 | 2008.8 | 8.1 | 75-00-3 | 1000 ppm (2600mg/m3/8H) | N/A |
| 3. Chloromethane | 79 | 06908MS | 2000 | 99.5 | 0.2 | 1.00508 | 1.0154 | 2020.5 | 8.1 | 74-87-3 | 100 ppm | ori-rat 1800mg/kg |
| 4. Dichlorodifluoromethane | 134 | 92-0487 | 2000 | 99 | 0.2 | 1.01016 | 1.0224 | 2024.2 | 8.2 | 75-71-8 | 1000 ppm (4950mg/m3/8H) | N/A |
| 5. Trichlorofluoromethane | 294 | 01823MW | 2000 | 99 | 0.2 | 1.01016 | 1.0110 | 2001.7 | 8.1 | 75-69-4 | 1000 ppm (5600mg/m3/8H) | ipr-mus 1743mg/kg |
| 6. Vinyl chloride | 305 | 04854EA | 2000 | 99.5 | 0.2 | 1.00508 | 1.0071 | 2004.0 | 8.1 | 75-01-4 | N/A | N/A |

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments

GC15-M9 Analysis by Melissa Stonier
Column ID SPB-Vocool 105 meter X 0.53mm X 3.0µm film thickness
Flow rates: Total flow=150mL/min., Helium (carrier)=10mL/min., Helium(make-up)=40mL/min., Hydrogen(make-up)=100mL/min.
Oven Profile: Temp. 1=35°C (Time 1=9 min.), Temp 2=200°C (Time 2=1 min.), Rate = 33°C/min., Total run time=15 min. Injector temp.=200°C, FID Temp.=200°C.
ELCD Signal = Edaq Channel 1 PID Signal = Edaq Channel 2
Standard injection = 0.5µL, Range=3 Purge Valve = 0 min.



| Peak No. | Analyte | ELCD RT (min.) |
|----------|-------------------------|----------------|
| 1 | Dichlorodifluoromethane | 4.67 |
| 2 | Chloromethane | 5.28 |
| 3 | Vinyl chloride | 5.56 |
| 4 | Bromomethane | 6.75 |
| 5 | Chloroethane | 6.99 |
| 6 | Trichlorofluoromethane | 7.72 |

ID #: 14285

Opened: _____
EPA Method 502-524 - Volatile Gases Mix #1
Expires: 8/3/2024
Rec'd: 9/17/2021
Energy Laboratories Inc 1120 So. 27th Street
Billings MT 59107

660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599
1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729
info@chemservice.com • www.chemservice.com

ID #: 14443

Opened: _____

TCL Ketone Mix

Expires: 6/30/2023

Rec'd: 10/26/2021

Energy Laboratories Inc 1120 So. 27th Street
Billings MT 59107

CERTIFICATE OF ANALYSIS

TCL Ketones Mixture

CONCENTRATION 2000ug/ml in Methanol:Water (90:10)
CATALOG NUMBER M-TCL1AN5-1ML
LOT NUMBER 10251200
DATE CERTIFIED 06/16/20
EXPIRATION DATE 06/30/23
STORAGE Freezer storage (-20 - -25 °C)
HANDLING See Safety Data Sheet
INTENDED USE For laboratory use only.
ISO 17034:2016 CERTIFIED []

| ID | Analyte | CAS | Weight Analyte (mg) | Lot | Purity | Certified Concentration (ug/mL) |
|---------|----------------------|----------|---------------------|----------|--------|---------------------------------|
| N-11014 | Acetone | 67-64-1 | 203.300 | 00026182 | 98.7 | 2006.6 |
| N-10297 | 2-Butanone | 78-93-3 | 202.800 | 00027454 | 99.5 | 2017.9 |
| N-10369 | 2-Hexanone | 591-78-6 | 202.600 | 00025720 | 99.5 | 2015.9 |
| N-10844 | 4-Methyl-2-pentanone | 108-10-1 | 204.700 | 6403300 | 99.5 | 2036.8 |

| Analytical Test | Value |
|------------------------|----------|
| CONCENTRATION (GC/FID) | VERIFIED |

Chem Service, Inc. is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015.



COA Form
Revision 3 (3/2015)

Print Date: 10/22/21

660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599
1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729
info@chemservice.com • www.chemservice.com

Instructions for Use:

Shake mixture prior to use. If particles are present, sonicate for homogeneity. If sample is diluted to lower concentrations, Class A volumetric glassware must be used.

Minimum Sample Size- 0.2 uL for Direct Injection.

Chem Service Inc. guarantees the expanded uncertainty of the above analytes to be +/- 2.0% of the certified concentrations based on gravimetric preparation. The test results published in this report were obtained using equipment capable of producing results that are traceable to NIST and through NIST to the International System of Units (SI). The reported expanded uncertainty of measurement is stated as the combined standard uncertainty of measurement multiplied by the coverage factor k (k=2) such that the coverage probability corresponds to approximately 95%. For certified reference materials, homogeneity and thermal stability testing are available upon request.

Certified By:

Mary Beth O'Donnell

Mary Beth O'Donnell
CSM/TC


Chem Service, Inc. is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015.



CERTIFICATE OF ANALYSIS

Gas Chromatography / Flame Ionization Detector (GC/FID)

Data file: C:\CHEM321\DATA\2020 DATA\0620M-TCL1AN5.D
 Sample name: M-TCL1AN5
 Acq. method: N-14278.M
 Instrument: GC3
 Injection date: 6/16/2020 2:52:35 PM
 Column name: RTX-5MS (30m x 0.25mm x 0.5µm)
 Location: 202
 Injection Vol: 1.000
 # Of Injections: 1



Signal: FID1 B, Back - Front Signal

| RT [min] | Type | Width [min] | Area | Height | Area% |
|-----------|------|-------------|----------|----------|---------|
| 2.592 | BB | 0.0277 | 580.2505 | 343.4986 | 18.4655 |
| 3.763 | BB | 0.0323 | 735.4804 | 387.8491 | 23.4054 |
| 6.969 | BB | 0.0326 | 904.3389 | 447.8770 | 28.7791 |
| 8.295 | BB | 0.0307 | 822.2798 | 474.3798 | 29.3500 |
| Sum | | | | | |
| 3142.3497 | | | | | |

Chem Service, Inc is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015.



CERTIFICATE OF ANALYSIS

Catalog No: CLP-022K-10X
Description: TCL Ketone Mix
Lot: 221101480
Solvent: Methanol
Hazards: Refer to SDS for complete safety information

Date Certified: Oct 26, 2021
Expiration: Nov 26, 2022
Sample Size: 1 mL
Components: 4
Storage Condition: Freeze (<-10 °C)



Certified Reference Material



| Component | CAS # | Purity % | Prepared Concentration ² | Certified Analyte Concentration ¹ |
|----------------------|----------|----------|-------------------------------------|--|
| | | (GC/MS) | (µg/mL) | (µg/mL) |
| Acetone | 67-64-1 | 100.0 | 2004 | 2004 |
| 2-Butanone | 78-93-3 | 100.0 | 2004 | 2004 |
| 2-Hexanone | 591-78-6 | 98.7 | 2004 | 1978 |
| 4-Methyl-2-pentanone | 108-10-1 | 100.0 | 2004 | 2004 |

ID #: 14567

Opened: _____
TCL Ketones Mixture
Expires: 11/26/2022
Rec'd: 11/30/2021
Energy Laboratories Inc 1120 So. 27th Street
Billings MT 59107

This Certified Reference Material was verified in accordance with ISO/IEC 17025

A product with a suffix (-1A, -2B, etc. or -01, -02, etc.) on its lot number has had its expiration date extended and is identical to the same lot number without the suffix.

² All weights are traceable through NIST, Test No. 684/289871-17

¹ Certified Analyte Concentration = Purity x Prepared Concentration.

The Uncertainty associated with the certified concentration reported on this certificate is $\pm 2.4\%$. This value is the combined expanded uncertainty and represents an estimated standard deviation equal to the positive square root of the total variation of the uncertainty of components. A normal distribution is assumed and a coverage factor of K=2 is chosen using approximately a 95% confidence level.

Labels and certificates follow U.S. Conventions in reporting numerical values: A comma (,) is used to separate units of one-thousand or greater. A period (.) is used as a decimal place marker.

The information on this certificate may not be reproduced without the express permission of the manufacturer. See reverse side for additional information

Hazard Information: Please refer to the SDS for information regarding the hazards associated with using this material.

This product was prepared according to in-house procedures and is guaranteed to be homogeneous.

Certified By: _____

Larry Decker, Organic QC Manager

CERTIFICATE OF ANALYSIS

Catalog No: CLP-022K-10X
Description: TCL Ketone Mix
Lot: 221101480
Solvent: Methanol

Date Certified: Oct 26, 2021
Expiration: Nov 26, 2022
Sample Size: 1 mL
Components: 4

T-Test

AccuStandard, Inc.
Statistical Report for CLP (SOW 1391)
26-Oct-2021

QR-QC-003 rev. 1/16

| RT Component | CLP-022K-10X 221101480 | | | | | | | CLP-022K-10X 221041075 | | | | | | | NOTES: | | | | | | |
|--------------------------------------|---------------------------|--------|--------|--------|------|---------|-------|---------------------------|--------|--------|--------|------|---------|-------|------------|-------|---------------------------------|------|-----------|---------------------------------|-----|
| | Run #1 | Run #2 | Run #3 | Run #4 | Mean | Std Dev | % RSD | Run #1 | Run #2 | Run #3 | Run #4 | Mean | Std Dev | % RSD | t.025 test | CI | Component | CI | # of Runs | 10 % error check of Conc. means | |
| 3.74 Acetone (67-64-1) | 1925 | 1881 | 1854 | 1803 | 1866 | 51.05 | 2.74% | 1751 | 1712 | 1730 | 1764 | 1764 | 22.43 | 1.29% | 4.36 | 119.2 | Acetone (67-64-1) | 56 | 4 | 2000 | 7 % |
| 5.77 2-Butanone (78-93-3) | 2275 | 2223 | 2237 | 2149 | 2221 | 52.79 | 2.38% | 2157 | 2103 | 2145 | 2177 | 2146 | 31.26 | 1.45% | 2.46 | 58.5 | 2-Butanone (78-93-3) | 35.9 | 4 | 2000 | 9 % |
| 8.34 4-Methyl-2-pentanone (108-10-1) | 3373 | 3302 | 3408 | 3225 | 3327 | 81.05 | 2.44% | 3349 | 3240 | 3296 | 3415 | 3325 | 74.70 | 2.25% | 0.04 | 0.9 | 4-Methyl-2-pentanone (108-10-1) | 0.8 | 4 | 2000 | 0 % |
| 9.13 2-Hexanone (99-178-6) | 3260 | 3199 | 3332 | 3118 | 3227 | 90.88 | 2.62% | 3186 | 3072 | 3120 | 3239 | 3154 | 73.32 | 2.32% | 1.25 | 35.2 | 2-Hexanone (99-178-6) | 29.1 | 4 | 2000 | 2 % |


CERTIFICATE OF ANALYSIS

Catalog No: CLP-022K-10X
Description: TCL Ketone Mix
Lot: 221101480
Solvent: Methanol


Date Certified: Oct 26, 2021
Expiration: Nov 26, 2022
Sample Size: 1 mL
Components: 4

Chromatogram

File : Q:\GCMS-06 Minimal\DATA\102521\13- 221101480 KM.D
Operator : Organic QC Lab
Acquired : 25 Oct 2021 21:00 using AcqMethod VOC-Split100.M
Instrument : GCMS 6
Sample Name : CLP-022K-10X (221101480)
Misc Info : TCL Ketone Mix @ 2000 ug/mL in MeOH
Vial Number: 34



Column: DB-624 UI, 30m x 0.25mm ID x 1.4µm
Oven Program: 35°C (hold 5min), 11°C/min to 60°C, 22°C/min to 230°C (hold 4min)
GC Parameters: Split 100:1, 1µl inj.; GC/MS; injector temp 240°C





Analytical RunID VOA5975C.I_220105A Standards Traceability Report

Standard ID: VOCF0313

Standard Name: Liquids

Prep Date: 6/23/2020

Exp Date: 4/13/2023

Department: gcmsvoa

Vendor: AccuStd

Lot Number: 220041126

Balance ID:

Comments: Date Prepared is same as Date Received. 2,000 ug/mL. Catalog # M502A-R-10X. Corrected lot number to match Cl. MSC 01/14/2022

Type: Primary

Prep By: Alethea M. Shaules

Status: New

Final Volume: 10 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|--------------------------------------|--------------|-----|-------|-----------|
| Volatile Organic Compounds - Liquids | <u>12797</u> | 1 | mL | 4/13/2023 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0313 | ug/mL | |



Analytical RunID VOA5975C.I_220105A Standards Traceability Report

Spike ID: VOCF0352

Spike Name: 2nd Source Liquids

Prep Date: 11/23/2020

Exp Date: 12/31/2023

Department: gcmsvoa

Vendor: Agilent

Lot Number: 0006570990

Balance ID:

Comments: Date Prepared is same as Date Received. 2000 ug/mL in MeOH. Catalog # DWM-589N-1.

Type: Primary

Prep By: Steve Dilts

Status: New

Final Volume: 10 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|-----------------------|--------------|-----|-------|------------|
| VOC Standard | <u>13292</u> | 1 | mL | 12/31/2023 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0352 | ug/mL | |



Analytical RunID VOA5975C.I_220105A Standards Traceability Report

Standard ID: VOCF0373

Standard Name: MtBE (Methy tert-Butyl Ether)

Prep Date: 2/26/2021

Exp Date: 8/31/2022

Department: gcmsvoa

Vendor: Agilent

Lot Number: 0006555762

Balance ID:

Comments: Date Prepared is same as Date Received. 2000 ug/mL in MeOH. Catalog # STS-440

Type: Primary

Prep By: Steve Dilts

Status: New

Final Volume: 5 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|----------------------------------|-----------|-----|-------|-----------|
| Methyl tert-Butyl Ether Standard | 13578 | 1 | mL | 8/31/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0373 | ug/mL | |



Analytical RunID VOA5975C.I_220105A Standards Traceability Report

Spike ID: VOCF0401

Spike Name: 2nd Source MtBE

Prep Date: 6/7/2021

Exp Date: 12/11/2029

Department: gcmsvoa

Vendor: AccuStandard

Lot Number: 220051182

Balance ID:

Comments: Date Prepared is same as Date Receive. 2,000 ug/mL in MeOH. Catalog # S-078-10X.

Type: Primary

Prep By: Alethea M. Shaules

Status: New

Final Volume: 5 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|-----------------------|-----------|-----|-------|------------|
| MTBE | 13920 | 1 | mL | 12/11/2029 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0401 | ug/mL | |



Analytical RunID VOA5975C.I_220105A Standards Traceability Report

Spike ID: VOCF0417

Spike Name: Chem Service Gases

Prep Date: 8/3/2021

Exp Date: 2/28/2022

Department: gcmsvoa

Vendor: Chemservice

Lot Number: 11882100

Balance ID:

Comments: Date Prepared is same as Date Received. 2000 ug/mL in MeOH. Catalog # M-VOHC6M5-1ML

Type: Primary

Prep By: Steve Dilts

Status: New

Final Volume: 5 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|---|--------------|-----|-------|-----------|
| Volatile Organics High Concentration Mixture #6 | <u>14142</u> | 5 | mL | 2/28/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0417 | ug/mL | |



Analytical RunID VOA5975C.I_220105A Standards Traceability Report

Standard ID: VOCF0425

Standard Name: Internals

Prep Date: 9/8/2021

Exp Date: 12/31/2022

Department: gcmsvoa

Vendor: Agilent

Lot Number: 0006582580

Balance ID:

Comments: Date Prepared is same as Date Received. 2,500 ug/mL in MeOH. Catalog # STM-520-1.

Type: Primary

Prep By: Jerran D. Brenden

Status: New

Final Volume: 10 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|-----------------------|--------------|-----|-------|------------|
| Internal Standard | <u>14251</u> | 1 | mL | 12/31/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0425 | ug/mL | |



Analytical RunID VOA5975C.I_220105A Standards Traceability Report

Spike ID: VOCF0426

Spike Name: Surrogates 2.0 mg/mL

Prep Date: 9/14/2021

Exp Date: 4/18/2029

Department: gcmsvoa

Vendor: AccuStandard

Lot Number: 219041458

Balance ID:

Comments: Date Received 01/04/2021. 2.0 mg/mL. Catalog # M-8260A-B-SS-10X

Type: Primary

Prep By: Jerran D. Brenden

Status: New

Final Volume: 10 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|------------------------|--------------|-----|-------|-----------|
| Surrogate Standard Mix | <u>14269</u> | 1 | mL | 4/18/2029 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0426 | ug/mL | |



Analytical RunID VOA5975C.I_220105A Standards Traceability Report

Standard ID: VOCF0427

Standard Name: Gases

Prep Date: 9/17/2021

Exp Date: 8/3/2024

Department: gcmsvoa

Vendor: Absolute

Lot Number: 080321

Balance ID:

Comments: Date Prepared is same as Date Received. 2,000 ug/mL in MeOH. Catalog # 30058.

Type: Primary

Prep By: Alethea M. Shaules

Status: New

Final Volume: 10 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|--|--------------|-----|-------|----------|
| EPA Method 502-524 - Volatile Gases Mix #1 | <u>14285</u> | 1 | mL | 8/3/2024 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0427 | ug/mL | |



Analytical RunID VOA5975C.I_220105A Standards Traceability Report

Standard ID: VOCF0434

Standard Name: Ketones

Prep Date: 10/26/2021

Exp Date: 6/30/2023

Department: gcmsvoa

Vendor: Chem Service

Lot Number: 10251200

Balance ID:

Comments: Date Prepared is same as Date Received. 2,000 ug/mL in 90:10 MeOH:H2O. Catalog # M-TCL-1AN5-5ML.

Type: Primary

Prep By: Steve Dilts

Status: New

Final Volume: 5 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|-----------------------|--------------|-----|-------|-----------|
| TCL Ketone Mix | <u>14443</u> | 1 | mL | 6/30/2023 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0434 | ug/mL | |



Analytical RunID VOA5975C.I_220105A Standards Traceability Report

Standard ID: VOCF0439

Standard Name: 2nd Source Ketones

Prep Date: 11/30/2021

Exp Date: 11/26/2022

Department: gcmsvoa

Vendor: AccuStandard

Lot Number: 221101480

Balance ID:

Comments: Date Prepared is same as Date Received. 2,000 ug/mL in Methanol. Catalog # CLP-022K-10X.

Type: Primary

Prep By: Melissa Chavez

Status: New

Final Volume: 1 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|-----------------------|--------------|-----|-------|------------|
| TCL Ketones Mixture | <u>14567</u> | 2 | mL | 11/26/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0439 | ug/mL | |



Analytical RunID VOA5975C.I_220105A Standards Traceability Report

Spike ID: VOCF3517

Spike Name: Internal Standard / Surrogates (INT/SURR)

Type: Secondary

Prep Date: 11/10/2021

Prep By: Alethea M. Shaules

Exp Date: 12/31/2022

Status: New

Department: gcmsvoa

Vendor:

Final Volume: 100 mL

Lot Number:

Balance ID:

Comments: Final Concentration 0.05 ug/uL in MeOH.

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|-------------------------------------|--------------|------|-------|------------|
| Methanol, Purge and Trap - EB199-US | <u>14334</u> | 95.5 | mL | 12/31/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0425 | ug/mL | 2 mL |
| VOCF0426 | ug/mL | 2.5 mL |



Analytical RunID VOA5975C.I_220105A Standards Traceability Report

Spike ID: VOCF3529B

Spike Name: 2nd Source MtBE

Prep Date: 11/29/2021

Exp Date: 1/29/2022

Department: gcmsvoa

Vendor:

Lot Number:

Balance ID:

Comments: Final Concentration 0.2 ug/uL

Type: Secondary

Prep By: Alethea M. Shaules

Status:

Final Volume: 10 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|-------------------------------------|--------------|-----|-------|-----------|
| Methanol, Purge and Trap - EB199-US | <u>14334</u> | 9 | mL | 1/29/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0401 | ug/mL | 1 mL |



Analytical RunID VOA5975C.I_220105A Standards Traceability Report

Standard ID: VOFC3546A

Standard Name: Liquids

Prep Date: 12/13/2021

Exp Date: 1/13/2022

Department: GCMSVOA

Vendor:

Lot Number:

Balance ID:

Comments: 1.0 ml/10 ml final volume. Final Concentration 0.2 ug/uL. Corrected comment and analyte list 11/9/2021 sbd

Type: Secondary

Prep By: Alethea M. Shaules

Status:

Final Volume: 10 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|--------------------------------|--------------|-----|-------|-----------|
| Methanol, Purge and Trap EA899 | <u>13926</u> | 9 | mL | 1/13/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0313 | ug/mL | 1 mL |



Analytical RunID VOA5975C.I_220105A Standards Traceability Report

Spike ID: VOCF3549

Spike Name: 2nd Source Ketones

Prep Date: 12/15/2021

Exp Date: 1/15/2022

Department: gcmsvoa

Vendor: AccuStandard

Lot Number: 221101480

Balance ID:

Comments: Vial opened for use. 2.0 µg/µL

Type: Primary

Prep By: Melissa Chavez

Status:

Final Volume: 1 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|-----------------------|--------------|-----|-------|-----------|
| TCL Ketones Mixture | <u>14567</u> | 1 | mL | 1/15/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0439 | ug/mL | 1 mL |



Analytical RunID VOA5975C.I_220105A Standards Traceability Report

Standard ID: VOFC3550

Standard Name: Ketones

Prep Date: 12/16/2021

Exp Date: 1/16/2022

Department: gcmsvoa

Vendor: Chem Service

Lot Number: 10251200

Balance ID:

Comments: Vial Opened For Use . 2.0 ug/uL in 90:10 MeOH:H2O.

Type: Primary

Prep By: Melissa Chavez

Status:

Final Volume: 1 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|-----------------------|--------------|-----|-------|-----------|
| TCL Ketone Mix | <u>14443</u> | 1 | mL | 1/16/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0434 | ug/mL | 1 mL |



Analytical RunID VOA5975C.I_220105A Standards Traceability Report

Spike ID: VOCF3558B

Spike Name: 2nd Source Liquids

Type: Secondary

Prep Date: 12/27/2021

Prep By: Steve Dilts

Exp Date: 2/27/2022

Status: Open

Department: gcmsvoa

Vendor:

Final Volume: 10 mL

Lot Number:

Balance ID:

Comments: Final Concentration 0.2ug/uL.

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|-------------------------------------|--------------|-----|-------|-----------|
| Methanol, Purge and Trap - EB199-US | <u>14334</u> | 9 | mL | 2/27/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0352 | ug/mL | 1 mL |



Analytical RunID VOA5975C.I_220105A Standards Traceability Report

Standard ID: VOCF3559A

Standard Name: MtBE

Prep Date: 12/27/2021

Exp Date: 1/27/2022

Department: gcmsvoa

Vendor:

Lot Number:

Balance ID:

Comments: Final Concentration 0.2 ug/uL.

Type: Secondary

Prep By: Melissa Chavez

Status:

Final Volume: 10 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|-------------------------------------|--------------|-----|-------|-----------|
| Methanol, Purge and Trap - EB199-US | <u>14334</u> | 9 | mL | 1/27/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0373 | ug/mL | 1 mL |



Analytical RunID VOA5975C.I_220105A Standards Traceability Report

Standard ID: VOCF3562A

Standard Name: Gases

Prep Date: 1/3/2022

Exp Date: 1/10/2022

Department: GCMSVOA

Vendor:

Lot Number:

Balance ID:

Comments: 1.0 ml/10 ml final volume. Final Concentration 0.2 ug/uL

Type: Secondary

Prep By: Alethea M. Shaules

Status:

Final Volume: 10 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|--------------------------------|--------------|-----|-------|-----------|
| Methanol, Purge and Trap EB373 | <u>14519</u> | 9 | mL | 1/10/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0427 | ug/mL | 1 mL |



Analytical RunID VOA5975C.I_220105A Standards Traceability Report

Spike ID: VO CF3566A

Spike Name: 2nd Source Gases

Prep Date: 1/4/2022

Exp Date: 1/11/2022

Department: gcmsvoa

Vendor:

Lot Number:

Balance ID:

Comments: 1.0 ml/10 ml final volume. Final Concentration 0.2 ug/uL. Corrected final volume column to match comments and added final concentrations of analytes. MSC 01/14/2021

Type: Secondary

Prep By: Melissa Chavez

Status:

Final Volume: 10 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires |
|--------------------------------|--------------|-----|-------|-----------|
| Methanol, Purge and Trap EB373 | <u>14519</u> | 9 | mL | 1/11/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0417 | ug/mL | 1 mL |

CERTIFICATE OF ANALYSIS

Catalog No: M-502A-R-10X
Description: Volatile Organic Compounds - Liquids
Lot: 220041126
Solvent: Methanol
Hazards: Refer to SDS for complete safety information

Date Certified: Apr 13, 2020
Expiration: Apr 13, 2023
Sample Size: 1 mL
Components: 54
Storage Condition: Refrig (0-5 °C)



Signal Word: Danger

Certified Reference Material



| Component | CAS # | Purity % (GC/MS) | Prepared Concentration* (µg/mL) | Certified Analyte Concentration* (µg/mL) |
|------------------------------|------------|---------------------|------------------------------------|---|
| Benzene | 71-43-2 | 100.0 | 2002 | 2002 |
| Bromobenzene | 108-86-1 | 100.0 | 2003 | 2003 |
| Bromochloromethane | 74-97-5 | 99.1 | 2001 | 1983 |
| Bromodichloromethane | 75-27-4 | 99.0 | 2002 | 1982 |
| Bromoform | 75-25-2 | 99.2 | 2001 | 1985 |
| n-Butylbenzene | 104-51-8 | 100.0 | 2002 | 2002 |
| sec-Butylbenzene | 135-98-8 | 100.0 | 2001 | 2001 |
| tert-Butylbenzene | 98-06-6 | 99.0 | 2003 | 1983 |
| Carbon tetrachloride | 56-23-5 | 100.0 | 2003 | 2003 |
| Chlorobenzene | 108-90-7 | 99.6 | 2001 | 1993 |
| Chloroform | 67-66-3 | 99.2 | 2004 | 1988 |
| 2-Chlorotoluene | 95-49-8 | 99.0 | 2003 | 1983 |
| 4-Chlorotoluene | 106-43-4 | 99.8 | 2002 | 1998 |
| Dibromochloromethane | 124-48-1 | 97.8 | 2049* | 2004 |
| 1,2-Dibromo-3-chloropropane | 96-12-8 | 99.2 | 2001 | 1985 |
| 1,2-Dibromoethane | 106-93-4 | 100.0 | 2006 | 2006 |
| Dibromomethane | 74-95-3 | 99.0 | 2002 | 1982 |
| 1,2-Dichlorobenzene | 95-50-1 | 98.2 | 2003 | 1967 |
| 1,3-Dichlorobenzene | 541-73-1 | 100.0 | 2000 | 2000 |
| 1,4-Dichlorobenzene | 106-46-7 | 100.0 | 2002 | 2002 |
| 1,1-Dichloroethane | 75-34-3 | 98.6 | 2001 | 1973 |
| 1,2-Dichloroethane | 107-06-2 | 99.8 | 2010 | 2006 |
| 1,1-Dichloroethene | 75-35-4 | 99.0 | 2000 | 1980 |
| cis-1,2-Dichloroethene | 156-59-2 | 99.0 | 2002 | 1982 |
| trans-1,2-Dichloroethene | 156-60-5 | 99.5 | 2001 | 1991 |
| 1,2-Dichloropropane | 78-87-5 | 99.5 | 2003 | 1993 |
| 1,3-Dichloropropane | 142-28-9 | 96.7 | 2073* | 2005 |
| 2,2-Dichloropropane | 594-20-7 | 99.9 | 2012 | 2010 |
| 1,1-Dichloropropene | 563-58-6 | 98.9 | 2001 | 1979 |
| cis-1,3-Dichloropropene ** | 10061-01-5 | 93.9 | 2041* | 1916 |
| trans-1,3-Dichloropropene ** | 10061-02-6 | 93.9 | 1968* | 1848 |
| Ethylbenzene | 100-41-4 | 99.7 | 2000 | 1994 |
| Hexachlorobutadiene | 87-68-3 | 98.0 | 2003 | 1963 |
| Isopropylbenzene | 98-82-8 | 100.0 | 2002 | 2002 |
| p-Isopropyltoluene | 99-87-6 | 99.4 | 2000 | 1988 |
| Methylene chloride | 75-09-2 | 99.9 | 2001 | 1999 |
| Naphthalene | 91-20-3 | 100.0 | 2002 | 2002 |
| n-Propylbenzene | 103-65-1 | 100.0 | 2001 | 2001 |
| Styrene | 100-42-5 | 100.0 | 2003 | 2003 |
| 1,1,1,2-Tetrachloroethane | 630-20-6 | 98.9 | 2005 | 1983 |
| 1,1,2,2-Tetrachloroethane | 79-34-5 | 96.0 | 2087* | 2004 |
| Tetrachloroethene | 127-18-4 | 99.4 | 2017 | 2005 |
| Toluene | 108-88-3 | 100.0 | 2001 | 2001 |
| 1,2,3-Trichlorobenzene | 87-61-6 | 100.0 | 2002 | 2002 |

CERTIFICATE OF ANALYSIS

Catalog No: M-502A-R-10X
Description: Volatile Organic Compounds - Liquids
Lot: 220041126
Solvent: Methanol

Date Certified: Apr 13, 2020
Expiration: Apr 13, 2023
Sample Size: 1 mL
Components: 54

| Component - <i>continued</i> | CAS # | Purity % | Prepared Concentration ² | Certified Analyte Concentration ¹ |
|------------------------------|----------|----------|-------------------------------------|--|
| | | (GC/MS) | (µg/mL) | (µg/mL) |
| 1,2,4-Trichlorobenzene | 120-82-1 | 99.6 | 2001 | 1993 |
| 1,1,1-Trichloroethane | 71-55-6 | 100.0 | 2002 | 2002 |
| 1,1,2-Trichloroethane | 79-00-5 | 98.6 | 2000 | 1972 |
| Trichloroethene | 79-01-6 | 100.0 | 2003 | 2003 |
| 1,2,3-Trichloropropane | 96-18-4 | 97.5 | 2055* | 2004 |
| 1,2,4-Trimethylbenzene | 95-63-6 | 98.2 | 2001 | 1965 |
| 1,3,5-Trimethylbenzene | 108-67-8 | 98.8 | 2001 | 1977 |
| o-Xylene | 95-47-6 | 99.0 | 2000 | 1980 |
| m-Xylene | 108-38-3 | 99.2 | 2002 | 1986 |
| p-Xylene | 106-42-3 | 95.4 | 2097* | 2001 |

* Weight compensated to 100% purity.

** 47.8% cis isomer, 46.1% trans isomer

A product with a suffix (-1A, -2B, etc. or -01, -02, etc.) on its lot number has had its expiration date extended and is identical to the same lot number without the suffix.

² All weights are traceable through NIST, Test No. 684/289871-17

¹ Certified Analyte Concentration = Purity x Prepared Concentration.

The Uncertainty associated with the certified concentration reported on this certificate is $\pm 2.4\%$. This value is the combined expanded uncertainty and represents an estimated standard deviation equal to the positive square root of the total variation of the uncertainty of components. A normal distribution is assumed and a coverage factor of K=2 is chosen using approximately a 95% confidence level.

Labels and certificates follow U.S. Conventions in reporting numerical values: A comma (,) is used to separate units of one-thousand or greater. A period (.) is used as a decimal place marker.

The information on this certificate may not be reproduced without the express permission of the manufacturer. See reverse side for additional information

Certified By:



Larry Decker, Organic QC Manager

ID #: 12797

Opened: _____

Volatile Organic Compounds - Liquids

Expires: 4/13/2023

Rec'd: 6/23/2020

Energy Laboratories Inc 1120 So. 27th Street
Billings MT 59107

Certificate of Analysis

Product Name: VOC Standard

Product Number: DWM-589N-1

Lot Number: 0006570990

Lot Issue Date: 17-Nov-2020

Expiration Date: 31-Dec-2023

Description:

This analytical reference material (RM) was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed below.

| Analyte | CAS# | Analyte Lot | Concentration ± Uncertainty |
|---------------------------|-------------|-------------|-----------------------------|
| bromochloromethane | 000074-97-5 | RM00009 | 2010 ± 10 µg/mL |
| bromodichloromethane | 000075-27-4 | RM12585 | 2009 ± 10 µg/mL |
| bromoform | 000075-25-2 | RM13987 | 2010 ± 10 µg/mL |
| carbon tetrachloride | 000056-23-5 | RM07576 | 2010 ± 10 µg/mL |
| chloroform | 000067-66-3 | RM13988 | 2009 ± 10 µg/mL |
| dibromochloromethane | 000124-48-1 | RM14843 | 2009 ± 10 µg/mL |
| dibromomethane | 000074-95-3 | RM12878 | 2009 ± 10 µg/mL |
| methylene chloride | 000075-09-2 | RM11650 | 2009 ± 10 µg/mL |
| 1,2-dibromoethane | 000106-93-4 | RM00018 | 2010 ± 10 µg/mL |
| 1,1-dichloroethane | 000075-34-3 | RM16217 | 2006 ± 10 µg/mL |
| 1,2-dichloroethane | 000107-06-2 | RM04655 | 2005 ± 10 µg/mL |
| 1,1-dichloroethene | 000075-35-4 | RM14486 | 2010 ± 10 µg/mL |
| cis-1,2-dichloroethene | 000156-59-2 | RM15008 | 2007 ± 10 µg/mL |
| trans-1,2-dichloroethene | 000156-60-5 | RM07565 | 2008 ± 10 µg/mL |
| 1,1,1,2-tetrachloroethane | 000630-20-6 | RM12632 | 2005 ± 10 µg/mL |
| 1,1,2,2-tetrachloroethane | 000079-34-5 | RM02540 | 2009 ± 10 µg/mL |
| tetrachloroethene | 000127-18-4 | RM06491 | 2008 ± 10 µg/mL |

Certificate of Analysis

| | | | |
|-----------------------------|-------------|--------------------|-----------------|
| Product Number: | DWM-589N-1 | Lot Number: | 0006570990 |
| 1,1,1-trichloroethane | 000071-55-6 | RM16539 | 2004 ± 10 µg/mL |
| 1,1,2-trichloroethane | 000079-00-5 | RM01175 | 2009 ± 10 µg/mL |
| trichloroethene | 000079-01-6 | RM14232 | 2009 ± 10 µg/mL |
| 1,2-dibromo-3-chloropropane | 000096-12-8 | RM13666 | 2009 ± 10 µg/mL |
| 1,2-dichloropropane | 000078-87-5 | RM12821 | 2008 ± 10 µg/mL |
| 1,3-dichloropropane | 000142-28-9 | RM02080 | 2008 ± 10 µg/mL |
| 2,2-dichloropropane | 000594-20-7 | RM12927 | 2005 ± 10 µg/mL |
| 1,1-dichloropropene | 000563-58-6 | RM16190 | 2010 ± 10 µg/mL |
| cis-1,3-dichloropropene | 010061-01-5 | RM12891 | 2007 ± 10 µg/mL |
| trans-1,3-dichloropropene | 010061-02-6 | RM12254 | 2006 ± 10 µg/mL |
| hexachlorobutadiene | 000087-68-3 | RM09157 | 2005 ± 10 µg/mL |
| 1,2,3-trichloropropane | 000096-18-4 | RM13082 | 2004 ± 10 µg/mL |
| benzene | 000071-43-2 | RM12931 | 2009 ± 10 µg/mL |
| n-butylbenzene | 000104-51-8 | RM03651 | 2008 ± 10 µg/mL |
| sec-butylbenzene | 000135-98-8 | RM10905 | 2005 ± 10 µg/mL |
| tert-butylbenzene | 000098-06-6 | RM14040 | 2007 ± 10 µg/mL |
| ethylbenzene | 000100-41-4 | RM12195 | 2006 ± 10 µg/mL |
| isopropylbenzene | 000098-82-8 | RM00835 | 2009 ± 10 µg/mL |
| 4-isopropyltoluene | 000099-87-6 | RM09747 | 2009 ± 10 µg/mL |
| naphthalene | 000091-20-3 | NT00970 | 2006 ± 10 µg/mL |
| n-propylbenzene | 000103-65-1 | RM12785 | 2010 ± 10 µg/mL |
| styrene | 000100-42-5 | RM13393 | 2010 ± 10 µg/mL |



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality Management System. Cert # 56 100 18560026

Page: 2 of 4

www.agilent.com/quality/
CSD-QA-015.1



ISO 17025 Cert
No. AT-1937



Certificate of Analysis

Product Number: DWM-589N-1

Lot Number: 0006570990

| | | | |
|------------------------|-------------|---------|-----------------|
| toluene | 000108-88-3 | RM06650 | 2008 ± 10 µg/mL |
| 1,2,4-trimethylbenzene | 000095-63-6 | RM06731 | 2002 ± 10 µg/mL |
| 1,3,5-trimethylbenzene | 000108-67-8 | RM12905 | 2009 ± 10 µg/mL |
| o-xylene | 000095-47-6 | RM15639 | 2005 ± 10 µg/mL |
| m-xylene | 000108-38-3 | RM15919 | 2006 ± 10 µg/mL |
| p-xylene | 000106-42-3 | RM02647 | 2009 ± 10 µg/mL |
| bromobenzene | 000108-86-1 | RM10227 | 2008 ± 10 µg/mL |
| chlorobenzene | 000108-90-7 | RM01874 | 2008 ± 10 µg/mL |
| 2-chlorotoluene | 000095-49-8 | RM13774 | 2007 ± 10 µg/mL |
| 4-chlorotoluene | 000106-43-4 | RM11750 | 2009 ± 10 µg/mL |
| 1,2-dichlorobenzene | 000095-50-1 | RM13636 | 2005 ± 10 µg/mL |
| 1,3-dichlorobenzene | 000541-73-1 | NT00356 | 2009 ± 10 µg/mL |
| 1,4-dichlorobenzene | 000106-46-7 | RM12826 | 2009 ± 10 µg/mL |
| 1,2,3-trichlorobenzene | 000087-61-6 | RM10193 | 2007 ± 10 µg/mL |
| 1,2,4-trichlorobenzene | 000120-82-1 | RM09454 | 2009 ± 10 µg/mL |

Matrix: methanol (methyl alcohol)

Storage Conditions: Store Frozen (-25° to -10°C).

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCCL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This RM was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality Management System. Cert # 56 100 18560026

Page: 3 of 4

www.agilent.com/quality/
CSD-QA-015.1



ISO 17025 Cert
No. AT-1937

Certificate of Analysis

Product Number: DWM-589N-1

Lot Number: 0006570990

Intended Use:

This RM is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Hazards:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this RM.


Expiration of Certification:

The certification of this RM is valid until the expiration date specified above, provided the RM is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the RM is damaged, contaminated, or otherwise modified.

Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:



Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality Management System. Cert # 56 100 18560026

Page: 4 of 4

www.agilent.com/quality/
CSD-QA-015.1



ISO 17025 Cert
No. AT-1937

Certificate of Analysis

Product Name: Methyl tert-Butyl Ether Standard**Product Number:** STS-440-1**Lot Number:** 0006555762**Lot Issue Date:** 19-Aug-2020**Expiration Date:** 31-Aug-2022**Description:**

This analytical reference material (RM) was manufactured and verified in accordance with an ISO 9001 registered quality system, and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed below.

Analyte**CAS#****Analyte Lot****Concentration ± Uncertainty**

tert-butylmethyl ether

001634-04-4

RM06568

2006 ± 10 µg/mL

Matrix: methanol (methyl alcohol)**Storage Conditions:** Store Frozen (-25° to -10°C).**Traceability:**

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCCL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This RM was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Intended Use:

This RM is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Hazards:


Refer to the Safety Data Sheet on www.agilent.com for information regarding this RM.

Expiration of Certification:

The certification of this RM is valid until the expiration date specified above, provided the RM is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the RM is damaged, contaminated, or otherwise modified.

Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:

Monica Bourgeois

QMS Representative

ISO 17034 Cert
No. AR-1936RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality
Management System. Cert # 56 100 18560026

Page: 1 of 1

www.agilent.com/quality/
CSD-QA-015.1ISO 17025 Cert
No. AT-1937

CERTIFICATE OF ANALYSIS

Catalog No: S-078-10X

Description: MtBE

Lot: 220051182

Solvent: Methanol

Hazards: Refer to SDS for complete safety information

Date Certified: May 18, 2020

Expiration: May 18, 2030

Sample Size: 1 mL

Components: 1

Storage Condition: Ambient (>5 °C)



Signal Word: Danger

Certified Reference Material



| Component | CAS # | Purity % (GC/MS) | Prepared Concentration ² (µg/mL) | Certified Analyte Concentration ¹ (µg/mL) |
|-----------|-----------|---------------------|--|---|
| MtBE | 1634-04-4 | 100.0 | 2002 | 2002 |

ID #: 13920

Opened: _____

MTBE

Expires: 5/18/2030

Rec'd: 6/7/2021

Eneray Laboratories Inc 1120 So. 27th Street
Billings MT 59107

A product with a suffix (-1A, -2B, etc. or -01, -02, etc.) on its lot number has had its expiration date extended and is identical to the same lot number without the suffix.

² All weights are traceable through NIST, Test No. 684/289871-17

¹ Certified Analyte Concentration = Purity x Prepared Concentration.

The Uncertainty associated with the certified concentration reported on this certificate is $\pm 2.4\%$. This value is the combined expanded uncertainty and represents an estimated standard deviation equal to the positive square root of the total variation of the uncertainty of components. A normal distribution is assumed and a coverage factor of K=2 is chosen using approximately a 95% confidence level.

Labels and certificates follow U.S. Conventions in reporting numerical values: A comma (,) is used to separate units of one-thousand or greater. A period (.) is used as a decimal place marker.

The information on this certificate may not be reproduced without the express permission of the manufacturer. See reverse side for additional information

Hazard Information: Please refer to the SDS for information regarding the hazards associated with using this material.

This product was prepared according to in-house procedures and is guaranteed to be homogeneous.

Certified By: _____

Larry Decker, Organic QC Manager

CERTIFICATE OF ANALYSIS

Volatile Organics High Concentration Mixture #6

CONCENTRATION 2000ug/ml in Methanol
CATALOG NUMBER M-VOHC6M5-1ML
LOT NUMBER 11882100
DATE CERTIFIED 05/25/21
EXPIRATION DATE 02/28/22
STORAGE Store at room temperature (20 - 25 °C).
HANDLING See Safety Data Sheet
INTENDED USE For laboratory use only.
ISO 17034:2016 CERTIFIED []

ID #: 14142

Opened:

Volatile Organics High Concentration Mixture

Expires: 2/28/2022

Rec'd: 8/3/2021

Energx Laboratories Inc 1120 So. 27th Street
Billings MT 59107

| ID | Analyte | CAS | Weight Analyte (mg) | Lot | Purity | Certified Concentration (ug/mL) |
|---------|-------------------------|---------|---------------------|----------|--------|---------------------------------|
| N-11446 | Chloroethane | 75-00-3 | 96.300 | 00001728 | 100.0 | 2006.3 |
| N-11665 | Dichlorodifluoromethane | 75-71-8 | 96.610 | 00001729 | 100.0 | 2012.7 |
| N-12417 | Methyl bromide | 74-83-9 | 96.910 | 00024694 | 100.0 | 2019.0 |
| N-12421 | Methyl chloride | 74-87-3 | 96.150 | 00001731 | 100.0 | 2003.1 |
| N-13655 | Trichlorofluoromethane | 75-69-4 | 96.300 | 00027239 | 99.4 | 1994.2 |
| N-13748 | Vinyl chloride | 75-01-4 | 96.150 | 00019298 | 100.0 | 2003.1 |

Analytical Test

Value

CONCENTRATION (GC/MSD)

VERIFIED

CHEM SERVICE INC

660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599
1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729
info@chemservice.com • www.chemservice.com

Instructions for Use:

Shake mixture prior to use. If particles are present, sonicate for homogeneity. If sample is diluted to lower concentrations, Class A volumetric glassware must be used.

Minimum Sample Size- 0.2 uL for Direct Injection.

Chem Service Inc. guarantees the expanded uncertainty of the above analytes to be +/- 2.0% of the certified concentrations based on gravimetric preparation. The test results published in this report were obtained using equipment capable of producing results that are traceable to NIST and through NIST to the International System of Units (SI). The reported expanded uncertainty of measurement is stated as the combined standard uncertainty of measurement multiplied by the coverage factor k (k=2) such that the coverage probability corresponds to approximately 95%. For certified reference materials, homogeneity and thermal stability testing are available upon request.

Certified By:

Mary Beth O'Donnell



Mary Beth O'Donnell
CSM/TC



CERTIFICATE OF ANALYSIS

Analysis Method:

Catalog Number: M-VOHC6M5-1ML
Description: Volatile Organics High Concentration Mixture #6
Lot Number: 11882100
Expiration Date: 02/28/22





Certificate of Analysis

ID #: 14251

Opened: _____

Internal Standard

Expires: 12/31/2022

Rec'd: 9/8/2021

Energy Laboratories Inc 1120 So. 27th Street
Billings MT 59107

Product Name: Internal Standard

Product Number: STM-520-1

Lot Issue Date: 05-Jan-2021

Lot Number: 0006582580

Expiration Date: 31-Dec-2022

Description:

This analytical reference material (RM) was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed below.

| Analyte | CAS# | Analyte Lot | Concentration ± Uncertainty |
|------------------------|-------------|-------------|-----------------------------|
| chlorobenzene-d5 | 003114-55-4 | RM12274 | 2501 ± 13 µg/mL |
| 1,4-dichlorobenzene-d4 | 003855-82-1 | RM12517 | 2501 ± 13 µg/mL |
| fluorobenzene | 000462-06-6 | RM13378 | 2512 ± 13 µg/mL |

Matrix: methanol (methyl alcohol)

Storage Conditions: Store Frozen (-25° to -10°C).

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCCL Z540.3, ISO 9001, ISO 17025 and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This RM was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Intended Use:

This RM is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Hazards:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this RM.



ISO 17034
REFERENCE MATERIAL
PRODUCER
ISO 17034 Cert
No. AR-1936

RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality Management System. Cert # 56 100 18560026

Page: 1 of 2

www.agilent.com/quality/
CSD-QA-015.1



ISO 17025 Cert
No. AT-1937



Certificate of Analysis

Product Number: STM-520-1

Lot Number: 0006582580

Expiration of Certification:

The certification of this RM is valid until the expiration date specified above, provided the RM is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the RM is damaged, contaminated, or otherwise modified.

Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:

Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality Management System. Cert # 56 100 18560026

Page: 2 of 2

www.agilent.com/quality/
CSD-QA-015.1



ISO 17025 Cert
No. AT-1937

CERTIFICATE OF ANALYSIS

Catalog No: M-8260A-B-SS-10X
Description: Surrogate Standard Mix
Lot: 219041458

Solvent: Methanol

Hazards: Refer to SDS for complete safety information

Date Certified: Apr 18, 2019

Expiration: Apr 18, 2029

Sample Size: 1 mL

Components: 4

Storage Condition: Ambient (>5 °C)



Signal Word: Danger

Certified Reference Material



| Component | CAS # | Purity % | Prepared | Certified Analyte |
|-----------------------|------------|----------|---------------------------------------|---------------------------------------|
| | | (GC/MS) | Concentration ² (µg/mL) | Concentration ¹ (µg/mL) |
| p-Bromofluorobenzene | 460-00-4 | 99.9 | 2004 | 2002 |
| Dibromofluoromethane | 1868-53-7 | 99.8 | 2005 | 2001 |
| 1,2-Dichloroethane-d4 | 17060-07-0 | 100.0 | 2001 | 2001 |
| Toluene-d8 | 2037-26-5 | 100.0 | 2000 | 2000 |

ID #: 14269

Opened: _____

Surrogate Standard Mix

Expires: 4/18/2029

Rec'd: 9/14/2021

Energy Laboratories Inc 1120 So. 27th Street
Billings MT 59107

A product with a suffix (-1A, -2B, etc. or -01, -02, etc.) on its lot number has had its expiration date extended and is identical to the same lot number without the suffix.

² All weights are traceable through NIST, Test No. 684/289871-17

¹ Certified Analyte Concentration = Purity x Prepared Concentration.

The Uncertainty associated with the certified concentration reported on this certificate is $\pm 2.4\%$. This value is the combined expanded uncertainty and represents an estimated standard deviation equal to the positive square root of the total variation of the uncertainty of components. A normal distribution is assumed and a coverage factor of K=2 is chosen using approximately a 95% confidence level.

Labels and certificates follow U.S. Conventions in reporting numerical values: A comma (,) is used to separate units of one-thousand or greater. A period (.) is used as a decimal place marker.



The information on this certificate may not be reproduced without the express permission of the manufacturer. See reverse side for additional information

Hazard Information: Please refer to the SDS for information regarding the hazards associated with using this material.

This product was prepared according to in-house procedures and is guaranteed to be homogeneous.

Certified By: _____

Larry Decker, Organic QC Manager



CERTIFIED WEIGHT REPORT

Part Number: 30058
Lot Number: 080321
Description: EPA Method 502/524 - Volatile Gases Mix #1
6 components
Expiration Date: 080324
Recommended Storage: Freezer (0 °C)
Nominal Concentration (µg/mL): 2000
NIST Test ID#: 6UTB
Solvent: Methanol
Lot#: EA783-US
5E-05 Balance Uncertainty
Weight(s) shown below were combined and diluted to (mL): 500.0 0.058 Flask Uncertainty


| | | |
|----------------|-----------------|--------|
| | | 080321 |
| Formulated By: | Mario Luis | DATE |
| | | 080321 |
| Reviewed By: | Pedro L. Rentas | DATE |

| Compound | RM# | Lot Number | Nominal Conc (µg/mL) | Purity (%) | Uncertainty Purity (%) | Target Weight (g) | Actual Weight (g) | Actual Conc(µg/mL) | Expanded Uncertainty (+/-) (µg/mL) | SDS Information (Solvent Safety Info. On Attached pg.) | | |
|----------------------------|-----|------------|----------------------|------------|------------------------|-------------------|-------------------|--------------------|------------------------------------|--|---------------------------|-------------------|
| | | | | | | | | | | CAS# | OSHA PEL (TWA) | LD50 |
| 1. Bromomethane | 50 | 01611JX | 2000 | 99.5 | 0.2 | 1.00508 | 1.0098 | 2009.4 | 8.1 | 74-83-9 | 5 ppm (20mg/m3/8H) (skin) | ori-rat 214mg/kg |
| 2. Chloroethane | 72 | 062617 | 2000 | 99 | 0.2 | 1.01016 | 1.0146 | 2008.8 | 8.1 | 75-00-3 | 1000 ppm (2600mg/m3/8H) | N/A |
| 3. Chloromethane | 79 | 06908MS | 2000 | 99.5 | 0.2 | 1.00508 | 1.0154 | 2020.5 | 8.1 | 74-87-3 | 100 ppm | ori-rat 1800mg/kg |
| 4. Dichlorodifluoromethane | 134 | 92-0487 | 2000 | 99 | 0.2 | 1.01016 | 1.0224 | 2024.2 | 8.2 | 75-71-8 | 1000 ppm (4950mg/m3/8H) | N/A |
| 5. Trichlorofluoromethane | 294 | 01823MW | 2000 | 99 | 0.2 | 1.01016 | 1.0110 | 2001.7 | 8.1 | 75-69-4 | 1000 ppm (5600mg/m3/8H) | ipr-mus 1743mg/kg |
| 6. Vinyl chloride | 305 | 04854EA | 2000 | 99.5 | 0.2 | 1.00508 | 1.0071 | 2004.0 | 8.1 | 75-01-4 | N/A | N/A |

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments

GC15-M9 Analysis by Melissa Stonier
Column ID SPB-Vocool 105 meter X 0.53mm X 3.0µm film thickness
Flow rates: Total flow=150mL/min., Helium (carrier)=10mL/min., Helium(make-up)=40mL/min., Hydrogen(make-up)=100mL/min.
Oven Profile: Temp. 1=35°C (Time 1=9 min.), Temp 2=200°C (Time 2=1 min.), Rate = 33°C/min., Total run time=15 min., Injector temp.=200°C, FID Temp.=200°C.
ELCD Signal = Edaq Channel 1 PID Signal = Edaq Channel 2
Standard injection = 0.5µL, Range=3 Purge Valve = 0 min.



| Peak No. | Analyte | ELCD RT (min.) |
|----------|-------------------------|----------------|
| 1 | Dichlorodifluoromethane | 4.67 |
| 2 | Chloromethane | 5.28 |
| 3 | Vinyl chloride | 5.56 |
| 4 | Bromomethane | 6.75 |
| 5 | Chloroethane | 6.99 |
| 6 | Trichlorofluoromethane | 7.72 |

ID #: 14285

Opened: _____
EPA Method 502-524 - Volatile Gases Mix #1
Expires: 8/3/2024
Rec'd: 9/17/2021
Energy Laboratories Inc 1120 So. 27th Street
Billings MT 59107

660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599
1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729
info@chemservice.com • www.chemservice.com

ID #: 14443

Opened: _____

TCL Ketone Mix

Expires: 6/30/2023

Rec'd: 10/26/2021

Energy Laboratories Inc 1120 So. 27th Street
Billings MT 59107

CERTIFICATE OF ANALYSIS

TCL Ketones Mixture

CONCENTRATION 2000ug/ml in Methanol:Water (90:10)
CATALOG NUMBER M-TCL1AN5-1ML
LOT NUMBER 10251200
DATE CERTIFIED 06/16/20
EXPIRATION DATE 06/30/23
STORAGE Freezer storage (-20 - -25 °C)
HANDLING See Safety Data Sheet
INTENDED USE For laboratory use only.
ISO 17034:2016 CERTIFIED []

| ID | Analyte | CAS | Weight Analyte (mg) | Lot | Purity | Certified Concentration (ug/mL) |
|---------|----------------------|----------|---------------------|----------|--------|---------------------------------|
| N-11014 | Acetone | 67-64-1 | 203.300 | 00026182 | 98.7 | 2006.6 |
| N-10297 | 2-Butanone | 78-93-3 | 202.800 | 00027454 | 99.5 | 2017.9 |
| N-10369 | 2-Hexanone | 591-78-6 | 202.600 | 00025720 | 99.5 | 2015.9 |
| N-10844 | 4-Methyl-2-pentanone | 108-10-1 | 204.700 | 6403300 | 99.5 | 2036.8 |

| Analytical Test | Value |
|------------------------|----------|
| CONCENTRATION (GC/FID) | VERIFIED |

Chem Service, Inc. is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015.



COA Form
Revision 3 (3/2015)

Print Date: 10/22/21

660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599
1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729
info@chemservice.com • www.chemservice.com

Instructions for Use:

Shake mixture prior to use. If particles are present, sonicate for homogeneity. If sample is diluted to lower concentrations, Class A volumetric glassware must be used.

Minimum Sample Size- 0.2 uL for Direct Injection.

Chem Service Inc. guarantees the expanded uncertainty of the above analytes to be +/- 2.0% of the certified concentrations based on gravimetric preparation. The test results published in this report were obtained using equipment capable of producing results that are traceable to NIST and through NIST to the International System of Units (SI). The reported expanded uncertainty of measurement is stated as the combined standard uncertainty of measurement multiplied by the coverage factor k (k=2) such that the coverage probability corresponds to approximately 95%. For certified reference materials, homogeneity and thermal stability testing are available upon request.

Certified By:

Mary Beth O'Donnell

Mary Beth O'Donnell
CSM/TC


Chem Service, Inc. is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015.



CERTIFICATE OF ANALYSIS

Gas Chromatography / Flame Ionization Detector (GC/FID)

Data file: C:\CHEM321\DATA\2020 DATA\0620M-TCL1AN5.D
 Sample name: M-TCL1AN5
 Acq. method: N-14278.M
 Instrument: GC3
 Injection date: 6/16/2020 2:52:35 PM
 Column name: RTX-5MS (30m x 0.25mm x 0.5µm)
 Location: 202
 Injection Vol: 1.000
 # Of Injections: 1



Signal: FID1 B, Back - Front Signal

| RT [min] | Type | Width [min] | Area | Height | Area% |
|----------|------|-------------|-----------|----------|---------|
| 2.592 | BB | 0.0277 | 580.2505 | 343.4986 | 18.4655 |
| 3.763 | BB | 0.0323 | 735.4804 | 387.8491 | 23.4054 |
| 6.969 | BB | 0.0326 | 904.3389 | 447.8770 | 28.7791 |
| 8.285 | BB | 0.0307 | 822.2798 | 474.3798 | 29.3500 |
| Sum | | | | | |
| | | | 3142.3497 | | |

Chem Service, Inc is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015.



CERTIFICATE OF ANALYSIS

Catalog No: CLP-022K-10X
Description: TCL Ketone Mix
Lot: 221101480
Solvent: Methanol
Hazards: Refer to SDS for complete safety information

Date Certified: Oct 26, 2021
Expiration: Nov 26, 2022
Sample Size: 1 mL
Components: 4
Storage Condition: Freeze (<-10 °C)



Certified Reference Material



| Component | CAS # | Purity % | Prepared Concentration ² | Certified Analyte Concentration ¹ |
|----------------------|----------|----------|-------------------------------------|--|
| | | (GC/MS) | (µg/mL) | (µg/mL) |
| Acetone | 67-64-1 | 100.0 | 2004 | 2004 |
| 2-Butanone | 78-93-3 | 100.0 | 2004 | 2004 |
| 2-Hexanone | 591-78-6 | 98.7 | 2004 | 1978 |
| 4-Methyl-2-pentanone | 108-10-1 | 100.0 | 2004 | 2004 |

ID #: 14567

Opened: _____

TCL Ketones Mixture

Expires: 11/26/2022

Rec'd: 11/30/2021

Energy Laboratories Inc 1120 So. 27th Street
Billings MT 59107

This Certified Reference Material was verified in accordance with ISO/IEC 17025

A product with a suffix (-1A, -2B, etc. or -01, -02, etc.) on its lot number has had its expiration date extended and is identical to the same lot number without the suffix.

² All weights are traceable through NIST, Test No. 684/289871-17

¹ Certified Analyte Concentration = Purity x Prepared Concentration.

The Uncertainty associated with the certified concentration reported on this certificate is $\pm 2.4\%$. This value is the combined expanded uncertainty and represents an estimated standard deviation equal to the positive square root of the total variation of the uncertainty of components. A normal distribution is assumed and a coverage factor of K=2 is chosen using approximately a 95% confidence level.

Labels and certificates follow U.S. Conventions in reporting numerical values: A comma (,) is used to separate units of one-thousand or greater. A period (.) is used as a decimal place marker.

The information on this certificate may not be reproduced without the express permission of the manufacturer. See reverse side for additional information

Hazard Information: Please refer to the SDS for information regarding the hazards associated with using this material.

This product was prepared according to in-house procedures and is guaranteed to be homogeneous.

Certified By: _____

Larry Decker, Organic QC Manager

CERTIFICATE OF ANALYSIS

Catalog No: CLP-022K-10X
Description: TCL Ketone Mix
Lot: 221101480
Solvent: Methanol

Date Certified: Oct 26, 2021
Expiration: Nov 26, 2022
Sample Size: 1 mL
Components: 4

T-Test

AccuStandard, Inc.
Statistical Report for CLP (SOW 1391)
26-Oct-2021

QR-QC-003 rev. 1/16

| RT Component | CLP-022K-10X 221101480 | | | | | | | CLP-022K-10X 221041075 | | | | | | | NOTES: | | | | | | |
|--------------------------------------|---------------------------|--------|--------|--------|------|---------|-------|---------------------------|--------|--------|--------|------|---------|-------|------------|-------|---------------------------------|------|-----------|---------------------------------|-----|
| | Run #1 | Run #2 | Run #3 | Run #4 | Mean | Std Dev | % RSD | Run #1 | Run #2 | Run #3 | Run #4 | Mean | Std Dev | % RSD | t.025 test | CI | Component | CI | # of Runs | 10 % error check of Conc. means | |
| 3.74 Acetone (67-64-1) | 1925 | 1881 | 1854 | 1803 | 1866 | 51.05 | 2.74% | 1751 | 1712 | 1730 | 1764 | 1764 | 22.43 | 1.29% | 4.36 | 119.2 | Acetone (67-64-1) | 56 | 4 | 2000 | 7 % |
| 5.77 2-Butanone (78-93-3) | 2275 | 2223 | 2237 | 2149 | 2221 | 52.79 | 2.38% | 2157 | 2103 | 2145 | 2177 | 2146 | 31.26 | 1.45% | 2.46 | 58.5 | 2-Butanone (78-93-3) | 35.9 | 4 | 2000 | 9 % |
| 8.34 4-Methyl-2-pentanone (108-10-1) | 3373 | 3302 | 3408 | 3225 | 3327 | 81.05 | 2.44% | 3349 | 3240 | 3296 | 3415 | 3325 | 74.70 | 2.25% | 0.04 | 0.9 | 4-Methyl-2-pentanone (108-10-1) | 0.8 | 4 | 2000 | 0 % |
| 9.13 2-Hexanone (98-178-6) | 3260 | 3199 | 3332 | 3118 | 3227 | 90.88 | 2.62% | 3186 | 3072 | 3120 | 3239 | 3154 | 73.32 | 2.32% | 1.25 | 35.2 | 2-Hexanone (98-178-6) | 29.1 | 4 | 2000 | 2 % |


CERTIFICATE OF ANALYSIS

Catalog No: CLP-022K-10X
Description: TCL Ketone Mix
Lot: 221101480
Solvent: Methanol

Date Certified: Oct 26, 2021
Expiration: Nov 26, 2022
Sample Size: 1 mL
Components: 4

Chromatogram

File : Q:\GCMS-06 Minimal\DATA\102521\13- 221101480 KM.D
Operator : Organic QC Lab
Acquired : 25 Oct 2021 21:00 using AcqMethod VOC-Split100.M
Instrument : GCMS 6
Sample Name : CLP-022K-10X (221101480)
Misc Info : TCL Ketone Mix @ 2000 ug/mL in MeOH
Vial Number : 34



Column: DB-624 UI, 30m x 0.25mm ID x 1.4µm
Oven Program: 35°C (hold 5min), 11°C/min to 60°C, 22°C/min to 230°C (hold 4min)
GC Parameters: Split 100:1, 1µl inj.; GC/MS; injector temp 240°C

