

PREP BATCH REPORT

Prep Code: **SVOC-3510C-8270**
 Prep Batch **162701** Prep Temp: **NA °C**

Technician: **Ryan F. Bengel**
 Batch Units: **ML**

Prep Start Date: **1/4/2022 3:47:52 PM**
 Prep End Date: **1/7/2022 4:25:00 PM**

Sample ID	Matrix	pH	Initial Samp Amt	Sol Added	Sol Recovered	Final Vol (mL)	Factor	Balance	Prep Start Date	Prep End Date
MB-162701			1000	0	0	1.00	0.001		1/4/2022	1/7/2022
LCS-162701			1000	0	0	1.00	0.001		1/4/2022	1/7/2022
LCSD-162701			1000	0	0	1.00	0.001		1/4/2022	1/7/2022
LLCS-162701			1000	0	0	1.00	0.001		1/4/2022	1/7/2022
LLCSD-162701			1000	0	0	1.00	0.001		1/4/2022	1/7/2022
APP2A-162701			1000	0	0	1.00	0.001		1/4/2022	1/7/2022
APP2AD-162701			1000	0	0	1.00	0.001		1/4/2022	1/7/2022
B22010096-001C	Ground Water	6	1020	0	0	1.00	0.00098		1/4/2022	1/7/2022
	Sample was clear (1/2)									
B22010120-001C	Ground Water	6	1030	0	0	1.00	0.000971		1/4/2022	1/7/2022
	Sample was slightly cloudy (1/2)									
B22010134-001C	Ground Water	6	1000	0	0	1.00	0.001		1/5/2022	1/7/2022
	Sample was clear (1/2)									
B22010141-001C	Ground Water	6	990	0	0	1.00	0.00101		1/5/2022	1/7/2022
	Sample was clear (1/2)									
B22010142-001C	Ground Water	6	1020	0	0	1.00	0.00098		1/5/2022	1/7/2022
	Sample was clear (2/2)									
B22010143-001C	Ground Water	6	1050	0	0	1.00	0.000952		1/5/2022	1/7/2022
	Sample was clear (1/2)									
B22010145-001C	Ground Water	6	990	0	0	1.00	0.00101		1/5/2022	1/7/2022
	Sample was clear (2/2)									
B22010148-001C	Ground Water	6	1010	0	0	1.00	0.00099		1/5/2022	1/7/2022
	Sample was clear (1/2)									
B22010141-001CLMS	Ground Water	6	990	0	0	1.00	0.00101		1/5/2022	1/7/2022
	Sample was clear (2/2)									
B22010134-001CMS	Ground Water	6	970	0	0	1.00	0.00103		1/5/2022	1/7/2022
	Sample was clear (2/2)									

Number	Reagent Name	Exp Date	Amt
13124	Sulfuric Acid 2020070739	7/2/2022	2mL
13273	pH-indicator Strips 0-14 HC025486	9/30/2024	
14196	Dichloromethane EB867	6/18/2023	100,50
14647	Dichloromethane EC832	10/28/2023	

Spk ID	Spike Name	SampType	AmtAdd	Exp Date
FP211227 14446	DCM RINSED FILTER PAPER	ALL		4/6/2026
Sulfate 12/27/21 (Baked Sodium Sulfate	ALL	varies	11/29/2026
sv92616	APP2A/Acetone	APP2A/D	1.0 mL	9/24/2022
sv83418	Benzidines	LCS, MS	50 uL	3/17/2024
sv92710	LCS/Add Extractions	LCS, MS; LLCS/	1.0 mL; 5	1/14/2022
SVOC NaOH 122	10 N NaOH	MB, LCS, SAMP,	5 drops	7/31/2023
sv92712	LL BNA Surr	SAMP, LMS, LLC	100 uL	1/30/2022
sv92706	BNA Surr	SAMP, MB, LCS,	100 uL	3/31/2022

PREP BATCH REPORT

Prep Code: **SVOC-3510C-8270**
 Prep Batch **162701** Prep Temp: **NA °C**

Technician: **Ryan F. Bengel**
 Batch Units: **ML**

Prep Start Date: **1/4/2022 3:47:52 PM**
 Prep End Date: **1/7/2022 4:25:00 PM**

Sample ID	Matrix	pH	Initial Samp Amt	Sol Added	Sol Recovered	Final Vol (mL)	Factor	Balance	Prep Start Date	Prep End Date
B22010209-001C	Ground Water Sample was clear (1/2)	6	1040	0	0	1.00	0.000962		1/5/2022	1/7/2022
B22010211-001C	Ground Water Sample had a yellow tint (1/2)	6	940	0	0	1.00	0.00106		1/5/2022	1/7/2022
B22010212-001C	Ground Water Sample was clear (1/2)	6	1020	0	0	1.00	0.00098		1/5/2022	1/7/2022

Number	Reagent Name	Exp Date	
13124	Sulfuric Acid 2020070739	7/2/2022	2mL
13273	pH-indicator Strips 0-14 HC025486	9/30/2024	
14196	Dichloromethane EB867	6/18/2023	100,50
14647	Dichloromethane EC832	10/28/2023	

Spk ID	Spike Name	SampType	AmtAdd	Exp Date
FP211227 14446	DCM RINSED FILTER PAPER	ALL		4/6/2026
Sulfate 12/27/21 (Baked Sodium Sulfate	ALL	varies	11/29/2026
sv92616	APP11A/Acetone	APP2A/D	1.0 mL	9/24/2022
sv83418	Benzidines	LCS, MS	50 uL	3/17/2024
sv92710	LCS/Add Extractions	LCS, MS; LLCS/	1.0 mL; 5	1/14/2022
SVOC NaOH 122	10 N NaOH	MB, LCS, SAMP,	5 drops	7/31/2023
sv92712	LL BNA Surr	SAMP, LMS, LLC	100 uL	1/30/2022
sv92706	BNA Surr	SAMP, MB, LCS,	100 uL	3/31/2022

Energy Laboratories Inc

ANALYTICAL RUN Summary

06-Jan-22

Run ID SV5975.I_211228A

Run Start Date: 12/28/2021
Analyst: John P. Heine
Ical:
Column ID: ZB-SemiVolatiles
Comments:

Std ID	Std Name	Std Amount	Std Units	Samp Amount	Samp Units	SampType	Expiration Date
dcmsvoc13	DCM						11/17/2022
sv100210	BNA 2nd source 200ug/mL	2	ul	198	ul	ICV	1/15/2022
sv100506	BNA low 50 ug/mL	8	ul	192	ul	CCV	3/31/2022
sv100703	BNA Internals 2000 ug/mL	50	ul	50	ul	TUNE	5/31/2022
sv83311	DFTPP 1000 ug/mL	50	ul	50	ul	TUNE	10/31/2022

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14955036	Dec2801_D_TU	SVOC-8270-DF	TUNE	/5975.I\sh122821\	12/28/2021 5:06:	1	R372497		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
127, % of mass 198	A	%	49.1	49.1		100	0	0	0	0.01	0	49%	40	60	0%	
197, % of mass 198	A	%	0	0		100	0	0	0	0.01	0	0%	0	0.99	0%	
198, Base Peak	A	%	100	100		100	0	0	0	0.01	0	100%	100	100	0%	
199, % of mass 198	A	%	6.6	6.6		100	0	0	0	0.01	0	7%	5	9	0%	
275, % of mass 198	A	%	29.6	29.6		100	0	0	0	0.01	0	30%	10	30	0%	
365, % of mass 198	A	%	2.9	2.9		100	0	0	0	0.01	0	3%	1	99.99	0%	
441, % of mass 443	A	%	98.7	98.7		100	0	0	0	0.01	0	99%	0.01	150	0%	
442, % of mass 198	A	%	50.7	50.7		100	0	0	0	0.01	0	51%	40	100	0%	
443, % of mass 442	A	%	19.8	19.8		100	0	0	0	0.01	0	20%	17	23	0%	
51, % of mass 198	A	%	50.7	50.7		100	0	0	0	0.01	0	51%	30	60	0%	
68, % of mass 69	A	%	0	0		100	0	0	0	0.01	0	0%	0	1.99	0%	
70, % of mass 69	A	%	0.5	0.5		100	0	0	0	0.01	0	1%	0	1.99	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14955037	28-Dec-21_CAL	SVOC-8270-W-	ICAL	/5975.I\sh122821	12/28/2021 5:30:	1	R372497		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	10.05866	10.05866		10	0	0	0.0206	0.1	10	101%	80	120	0%	
2-Methylnaphthalene	A	ug/L	10.36924	10.36924		10	0	0	0.0176	0.1	10	104%	80	120	0%	
Acenaphthene	A	ug/L	8.95221	8.95221		10	0	0	0.0317	0.1	10	90%	80	120	0%	
Acenaphthylene	A	ug/L	9.66426	9.66426		10	0	0	0.025	0.1	10	97%	80	120	0%	
Anthracene	A	ug/L	10.01599	10.01599		10	0	0	0.0283	0.1	10	100%	80	120	0%	
Benzo(a)anthracene	A	ug/L	10.16112	10.16112		10	0	0	0.0272	0.1	10	102%	80	120	0%	
Benzo(a)pyrene	A	ug/L	10.03426	10.03426		10	0	0	0.0347	0.1	10	100%	80	120	0%	
Benzo(b)fluoranthene	A	ug/L	11.94645	11.94645		10	0	0	0.0226	0.1	10	119%	80	120	0%	
Benzo(g,h,i)perylene	A	ug/L	10.05348	10.05348		10	0	0	0.0267	0.1	10	101%	80	120	0%	
Benzo(k)fluoranthene	A	ug/L	10.01427	10.01427		10	0	0	0.0295	0.1	10	100%	80	120	0%	
Chrysene	A	ug/L	10.13124	10.13124		10	0	0	0.0458	0.1	10	101%	80	120	0%	
Dibenzo(a,h)anthracene	A	ug/L	11.37434	11.37434		10	0	0	0.0367	0.1	10	114%	80	120	0%	
Fluoranthene	A	ug/L	9.91111	9.91111		10	0	0	0.0233	0.1	10	99%	80	120	0%	
Fluorene	A	ug/L	9.76802	9.76802		10	0	0	0.0225	0.1	10	98%	80	120	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	11.76689	11.76689		10	0	0	0.0491	0.1	10	118%	80	120	0%	
Naphthalene	A	ug/L	10.51984	10.51984		10	0	0	0.029	0.1	10	105%	80	120	0%	
Phenanthrene	A	ug/L	10.15862	10.15862		10	0	0	0.0295	0.1	10	102%	80	120	0%	
Pyrene	A	ug/L	9.96572	9.96572		10	0	0	0.0239	0.1	10	100%	80	120	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
2-Fluorobiphenyl	S	ug/L	9.48944	9.48944		10	0	0	0.0444	0.1	10	95%	80	120	0%	
Nitrobenzene-d5	S	ug/L	9.96587	9.96587		10	0	0	0.0523	0.1	10	100%	80	120	0%	
Terphenyl-d14	S	ug/L	10.25802	10.25802		10	0	0	0.0563	0.1	10	103%	80	120	0%	
o-Terphenyl	X	ug/L	9.6658	9.6658		10	0	0	0.0654	0.1	10	97%	80	120	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14955038	28-Dec-21_CAL	SVOC-8270-W-	ICAL	/5975.I\sh122821	12/28/2021 6:03:	1	R372497		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14955038	28-Dec-21_CAL	SVOC-8270-W-	ICAL	/5975.I\sh122821	12/28/2021 6:03:	1	R372497		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	4.60268	4.60268		5	0	0	0.0206	0.1	10	92%	80	120	0%	
2-Methylnaphthalene	A	ug/L	4.56926	4.56926		5	0	0	0.0176	0.1	10	91%	80	120	0%	
Acenaphthene	A	ug/L	4.53675	4.53675		5	0	0	0.0317	0.1	10	91%	80	120	0%	
Acenaphthylene	A	ug/L	4.66606	4.66606		5	0	0	0.025	0.1	10	93%	80	120	0%	
Anthracene	A	ug/L	4.96885	4.96885		5	0	0	0.0283	0.1	10	99%	80	120	0%	
Benzo(a)anthracene	A	ug/L	4.81813	4.81813		5	0	0	0.0272	0.1	10	96%	80	120	0%	
Benzo(a)pyrene	A	ug/L	4.90298	4.90298		5	0	0	0.0347	0.1	10	98%	80	120	0%	
Benzo(b)fluoranthene	A	ug/L	5.18655	5.18655		5	0	0	0.0226	0.1	10	104%	80	120	0%	
Benzo(g,h,i)perylene	A	ug/L	4.84572	4.84572		5	0	0	0.0267	0.1	10	97%	80	120	0%	
Benzo(k)fluoranthene	A	ug/L	4.95002	4.95002		5	0	0	0.0295	0.1	10	99%	80	120	0%	
Chrysene	A	ug/L	4.85617	4.85617		5	0	0	0.0458	0.1	10	97%	80	120	0%	
Dibenzo(a,h)anthracene	A	ug/L	4.66455	4.66455		5	0	0	0.0367	0.1	10	93%	80	120	0%	
Fluoranthene	A	ug/L	4.60748	4.60748		5	0	0	0.0233	0.1	10	92%	80	120	0%	
Fluorene	A	ug/L	4.84804	4.84804		5	0	0	0.0225	0.1	10	97%	80	120	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	4.81923	4.81923		5	0	0	0.0491	0.1	10	96%	80	120	0%	
Naphthalene	A	ug/L	4.80181	4.80181		5	0	0	0.029	0.1	10	96%	80	120	0%	
Phenanthrene	A	ug/L	4.88339	4.88339		5	0	0	0.0295	0.1	10	98%	80	120	0%	
Pyrene	A	ug/L	4.48873	4.48873		5	0	0	0.0239	0.1	10	90%	80	120	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
2-Fluorobiphenyl	S	ug/L	4.608	4.608		5	0	0	0.0444	0.1	10	92%	80	120	0%	
Nitrobenzene-d5	S	ug/L	5.112	5.112		5	0	0	0.0523	0.1	10	102%	80	120	0%	
Terphenyl-d14	S	ug/L	4.6204	4.6204		5	0	0	0.0563	0.1	10	92%	80	120	0%	
o-Terphenyl	X	ug/L	4.51295	4.51295		5	0	0	0.0654	0.1	10	90%	80	120	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14955039	28-Dec-21_CAL	SVOC-8270-W-	ICAL	/5975.I\sh122821	12/28/2021 6:35:	1	R372497		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14955039	28-Dec-21_CAL	SVOC-8270-W-	ICAL	/5975.I\sh122821\	12/28/2021 6:35:	1	R372497		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	1.83681	1.83681		2	0	0	0.0206	0.1	10	92%	80	120	0%	
2-Methylnaphthalene	A	ug/L	1.87323	1.87323		2	0	0	0.0176	0.1	10	94%	80	120	0%	
Acenaphthene	A	ug/L	1.86231	1.86231		2	0	0	0.0317	0.1	10	93%	80	120	0%	
Acenaphthylene	A	ug/L	1.80027	1.80027		2	0	0	0.025	0.1	10	90%	80	120	0%	
Anthracene	A	ug/L	1.96434	1.96434		2	0	0	0.0283	0.1	10	98%	80	120	0%	
Benzo(a)anthracene	A	ug/L	1.94879	1.94879		2	0	0	0.0272	0.1	10	97%	80	120	0%	
Benzo(a)pyrene	A	ug/L	1.99973	1.99973		2	0	0	0.0347	0.1	10	100%	80	120	0%	
Benzo(b)fluoranthene	A	ug/L	1.92723	1.92723		2	0	0	0.0226	0.1	10	96%	80	120	0%	
Benzo(g,h,i)perylene	A	ug/L	2.02605	2.02605		2	0	0	0.0267	0.1	10	101%	80	120	0%	
Benzo(k)fluoranthene	A	ug/L	2.04865	2.04865		2	0	0	0.0295	0.1	10	102%	80	120	0%	
Chrysene	A	ug/L	1.95136	1.95136		2	0	0	0.0458	0.1	10	98%	80	120	0%	
Dibenzo(a,h)anthracene	A	ug/L	1.85378	1.85378		2	0	0	0.0367	0.1	10	93%	80	120	0%	
Fluoranthene	A	ug/L	1.78571	1.78571		2	0	0	0.0233	0.1	10	89%	80	120	0%	
Fluorene	A	ug/L	1.85037	1.85037		2	0	0	0.0225	0.1	10	93%	80	120	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	1.83434	1.83434		2	0	0	0.0491	0.1	10	92%	80	120	0%	
Naphthalene	A	ug/L	1.90307	1.90307		2	0	0	0.029	0.1	10	95%	80	120	0%	
Phenanthrene	A	ug/L	1.91502	1.91502		2	0	0	0.0295	0.1	10	96%	80	120	0%	
Pyrene	A	ug/L	1.82293	1.82293		2	0	0	0.0239	0.1	10	91%	80	120	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
2-Fluorobiphenyl	S	ug/L	1.81035	1.81035		2	0	0	0.0444	0.1	10	91%	80	120	0%	
Nitrobenzene-d5	S	ug/L	1.92078	1.92078		2	0	0	0.0523	0.1	10	96%	80	120	0%	
Terphenyl-d14	S	ug/L	1.83901	1.83901		2	0	0	0.0563	0.1	10	92%	80	120	0%	
o-Terphenyl	X	ug/L	1.75229	1.75229		2	0	0	0.0654	0.1	10	88%	80	120	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14955040	28-Dec-21_CAL	SVOC-8270-W-	ICAL	/5975.I\sh122821\	12/28/2021 7:08:	1	R372497		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14955040	28-Dec-21_CAL	SVOC-8270-W-	ICAL	/5975.I\sh122821\	12/28/2021 7:08:	1	R372497		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0.96704	0.96704		1	0	0	0.0206	0.1	10	97%	80	120	0%	
2-Methylnaphthalene	A	ug/L	0.98056	0.98056		1	0	0	0.0176	0.1	10	98%	80	120	0%	
Acenaphthene	A	ug/L	1.00021	1.00021		1	0	0	0.0317	0.1	10	100%	80	120	0%	
Acenaphthylene	A	ug/L	0.99766	0.99766		1	0	0	0.025	0.1	10	100%	80	120	0%	
Anthracene	A	ug/L	1.01153	1.01153		1	0	0	0.0283	0.1	10	101%	80	120	0%	
Benzo(a)anthracene	A	ug/L	1.03188	1.03188		1	0	0	0.0272	0.1	10	103%	80	120	0%	
Benzo(a)pyrene	A	ug/L	1.05124	1.05124		1	0	0	0.0347	0.1	10	105%	80	120	0%	
Benzo(b)fluoranthene	A	ug/L	0.93908	0.93908		1	0	0	0.0226	0.1	10	94%	80	120	0%	
Benzo(g,h,i)perylene	A	ug/L	1.05674	1.05674		1	0	0	0.0267	0.1	10	106%	80	120	0%	
Benzo(k)fluoranthene	A	ug/L	0.99256	0.99256		1	0	0	0.0295	0.1	10	99%	80	120	0%	
Chrysene	A	ug/L	1.03479	1.03479		1	0	0	0.0458	0.1	10	103%	80	120	0%	
Dibenzo(a,h)anthracene	A	ug/L	0.98326	0.98326		1	0	0	0.0367	0.1	10	98%	80	120	0%	
Fluoranthene	A	ug/L	0.96817	0.96817		1	0	0	0.0233	0.1	10	97%	80	120	0%	
Fluorene	A	ug/L	0.99949	0.99949		1	0	0	0.0225	0.1	10	100%	80	120	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	0.95175	0.95175		1	0	0	0.0491	0.1	10	95%	80	120	0%	
Naphthalene	A	ug/L	0.99085	0.99085		1	0	0	0.029	0.1	10	99%	80	120	0%	
Phenanthrene	A	ug/L	1.02051	1.02051		1	0	0	0.0295	0.1	10	102%	80	120	0%	
Pyrene	A	ug/L	0.94277	0.94277		1	0	0	0.0239	0.1	10	94%	80	120	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
2-Fluorobiphenyl	S	ug/L	0.98499	0.98499		1	0	0	0.0444	0.1	10	98%	80	120	0%	
Nitrobenzene-d5	S	ug/L	0.97822	0.97822		1	0	0	0.0523	0.1	10	98%	80	120	0%	
Terphenyl-d14	S	ug/L	0.95599	0.95599		1	0	0	0.0563	0.1	10	96%	80	120	0%	
o-Terphenyl	X	ug/L	0.96943	0.96943		1	0	0	0.0654	0.1	10	97%	80	120	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14955041	28-Dec-21_CAL	SVOC-8270-W-	ICAL	/5975.I\sh122821\	12/28/2021 7:41:	1	R372497		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14955041	28-Dec-21_CAL	SVOC-8270-W-	ICAL	/5975.I\sh122821\	12/28/2021 7:41:	1	R372497		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0.49798	0.49798		0.5	0	0	0.0206	0.1	10	100%	80	120	0%	
2-Methylnaphthalene	A	ug/L	0.52362	0.52362		0.5	0	0	0.0176	0.1	10	105%	80	120	0%	
Acenaphthene	A	ug/L	0.50987	0.50987		0.5	0	0	0.0317	0.1	10	102%	80	120	0%	
Acenaphthylene	A	ug/L	0.49082	0.49082		0.5	0	0	0.025	0.1	10	98%	80	120	0%	
Anthracene	A	ug/L	0.54952	0.54952		0.5	0	0	0.0283	0.1	10	110%	80	120	0%	
Benzo(a)anthracene	A	ug/L	0.52804	0.52804		0.5	0	0	0.0272	0.1	10	106%	80	120	0%	
Benzo(a)pyrene	A	ug/L	0.53728	0.53728		0.5	0	0	0.0347	0.1	10	107%	80	120	0%	
Benzo(b)fluoranthene	A	ug/L	0.46329	0.46329		0.5	0	0	0.0226	0.1	10	93%	80	120	0%	
Benzo(g,h,i)perylene	A	ug/L	0.54194	0.54194		0.5	0	0	0.0267	0.1	10	108%	80	120	0%	
Benzo(k)fluoranthene	A	ug/L	0.49222	0.49222		0.5	0	0	0.0295	0.1	10	98%	80	120	0%	
Chrysene	A	ug/L	0.53181	0.53181		0.5	0	0	0.0458	0.1	10	106%	80	120	0%	
Dibenzo(a,h)anthracene	A	ug/L	0.49819	0.49819		0.5	0	0	0.0367	0.1	10	100%	80	120	0%	
Fluoranthene	A	ug/L	0.49263	0.49263		0.5	0	0	0.0233	0.1	10	99%	80	120	0%	
Fluorene	A	ug/L	0.52342	0.52342		0.5	0	0	0.0225	0.1	10	105%	80	120	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	0.50221	0.50221		0.5	0	0	0.0491	0.1	10	100%	80	120	0%	
Naphthalene	A	ug/L	0.49743	0.49743		0.5	0	0	0.029	0.1	10	99%	80	120	0%	
Phenanthrene	A	ug/L	0.51828	0.51828		0.5	0	0	0.0295	0.1	10	104%	80	120	0%	
Pyrene	A	ug/L	0.50292	0.50292		0.5	0	0	0.0239	0.1	10	101%	80	120	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
2-Fluorobiphenyl	S	ug/L	0.49774	0.49774		0.5	0	0	0.0444	0.1	10	100%	80	120	0%	
Nitrobenzene-d5	S	ug/L	0.51973	0.51973		0.5	0	0	0.0523	0.1	10	104%	80	120	0%	
Terphenyl-d14	S	ug/L	0.49855	0.49855		0.5	0	0	0.0563	0.1	10	100%	80	120	0%	
o-Terphenyl	X	ug/L	0.49787	0.49787		0.5	0	0	0.0654	0.1	10	100%	80	120	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14955042	28-Dec-21_CAL	SVOC-8270-W-	ICAL	/5975.I\sh122821\	12/28/2021 8:13:	1	R372497		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14955042	28-Dec-21_CAL	SVOC-8270-W-	ICAL	/5975.I\sh122821\	12/28/2021 8:13:	1	R372497		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0.20662	0.20662		0.2	0	0	0.0206	0.1	10	103%	80	120	0%	
2-Methylnaphthalene	A	ug/L	0.20517	0.20517		0.2	0	0	0.0176	0.1	10	103%	80	120	0%	
Acenaphthene	A	ug/L	0.21999	0.21999		0.2	0	0	0.0317	0.1	10	110%	80	120	0%	
Acenaphthylene	A	ug/L	0.21233	0.21233		0.2	0	0	0.025	0.1	10	106%	80	120	0%	
Anthracene	A	ug/L	0.19983	0.19983		0.2	0	0	0.0283	0.1	10	100%	80	120	0%	
Benzo(a)anthracene	A	ug/L	0.18839	0.18839		0.2	0	0	0.0272	0.1	10	94%	80	120	0%	
Benzo(a)pyrene	A	ug/L	0.18096	0.18096		0.2	0	0	0.0347	0.1	10	90%	80	120	0%	
Benzo(b)fluoranthene	A	ug/L	0.18728	0.18728		0.2	0	0	0.0226	0.1	10	94%	80	120	0%	
Benzo(g,h,i)perylene	A	ug/L	0.18972	0.18972		0.2	0	0	0.0267	0.1	10	95%	80	120	0%	
Benzo(k)fluoranthene	A	ug/L	0.20506	0.20506		0.2	0	0	0.0295	0.1	10	103%	80	120	0%	
Chrysene	A	ug/L	0.18246	0.18246		0.2	0	0	0.0458	0.1	10	91%	80	120	0%	
Dibenzo(a,h)anthracene	A	ug/L	0.19922	0.19922		0.2	0	0	0.0367	0.1	10	100%	80	120	0%	
Fluoranthene	A	ug/L	0.21099	0.21099		0.2	0	0	0.0233	0.1	10	105%	80	120	0%	
Fluorene	A	ug/L	0.20067	0.20067		0.2	0	0	0.0225	0.1	10	100%	80	120	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	0.18454	0.18454		0.2	0	0	0.0491	0.1	10	92%	80	120	0%	
Naphthalene	A	ug/L	0.1946	0.1946		0.2	0	0	0.029	0.1	10	97%	80	120	0%	
Phenanthrene	A	ug/L	0.19993	0.19993		0.2	0	0	0.0295	0.1	10	100%	80	120	0%	
Pyrene	A	ug/L	0.20969	0.20969		0.2	0	0	0.0239	0.1	10	105%	80	120	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
2-Fluorobiphenyl	S	ug/L	0.21251	0.21251		0.2	0	0	0.0444	0.1	10	106%	80	120	0%	
Nitrobenzene-d5	S	ug/L	0.19989	0.19989		0.2	0	0	0.0523	0.1	10	100%	80	120	0%	
Terphenyl-d14	S	ug/L	0.2059	0.2059		0.2	0	0	0.0563	0.1	10	103%	80	120	0%	
o-Terphenyl	X	ug/L	0.21371	0.21371		0.2	0	0	0.0654	0.1	10	107%	80	120	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14955043	28-Dec-21_CAL	SVOC-8270-W-	ICAL	/5975.I\sh122821\	12/28/2021 8:46:	1	R372497		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14955043	28-Dec-21_CAL	SVOC-8270-W-	ICAL	/5975.I\sh122821	12/28/2021 8:46:	1	R372497		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0.11591	0.11591		0.1	0	0	0.0206	0.1	10	116%	50	150	0%	
2-Methylnaphthalene	A	ug/L	0.1059	0.1059		0.1	0	0	0.0176	0.1	10	106%	50	150	0%	
Acenaphthene	A	ug/L	0.11464	0.11464		0.1	0	0	0.0317	0.1	10	115%	50	150	0%	
Acenaphthylene	A	ug/L	0.11593	0.11593		0.1	0	0	0.025	0.1	10	116%	50	150	0%	
Anthracene	A	ug/L	0.09125	0.09125		0.1	0	0	0.0283	0.1	10	91%	50	150	0%	
Benzo(a)anthracene	A	ug/L	0.10164	0.10164		0.1	0	0	0.0272	0.1	10	102%	50	150	0%	
Benzo(a)pyrene	A	ug/L	0.09848	0.09848		0.1	0	0	0.0347	0.1	10	98%	50	150	0%	
Benzo(b)fluoranthene	A	ug/L	0.10024	0.10024		0.1	0	0	0.0226	0.1	10	100%	50	150	0%	
Benzo(g,h,i)perylene	A	ug/L	0.09225	0.09225		0.1	0	0	0.0267	0.1	10	92%	50	150	0%	
Benzo(k)fluoranthene	A	ug/L	0.09818	0.09818		0.1	0	0	0.0295	0.1	10	98%	50	150	0%	
Chrysene	A	ug/L	0.10293	0.10293		0.1	0	0	0.0458	0.1	10	103%	50	150	0%	
Dibenzo(a,h)anthracene	A	ug/L	0.1027	0.1027		0.1	0	0	0.0367	0.1	10	103%	50	150	0%	
Fluoranthene	A	ug/L	0.11861	0.11861		0.1	0	0	0.0233	0.1	10	119%	50	150	0%	
Fluorene	A	ug/L	0.10787	0.10787		0.1	0	0	0.0225	0.1	10	108%	50	150	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	0.10634	0.10634		0.1	0	0	0.0491	0.1	10	106%	50	150	0%	
Naphthalene	A	ug/L	0.10774	0.10774		0.1	0	0	0.029	0.1	10	108%	50	150	0%	
Phenanthrene	A	ug/L	0.09933	0.09933		0.1	0	0	0.0295	0.1	10	99%	50	150	0%	
Pyrene	A	ug/L	0.11971	0.11971		0.1	0	0	0.0239	0.1	10	120%	50	150	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
2-Fluorobiphenyl	S	ug/L	0.11813	0.11813		0.1	0	0	0.0444	0.1	10	118%	50	150	0%	
Nitrobenzene-d5	S	ug/L	0.10034	0.10034		0.1	0	0	0.0523	0.1	10	100%	50	150	0%	
Terphenyl-d14	S	ug/L	0.1148	0.1148		0.1	0	0	0.0563	0.1	10	115%	50	150	0%	
o-Terphenyl	X	ug/L	0.12209	0.12209		0.1	0	0	0.0654	0.1	10	122%	50	150	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14955044	28-Dec-21_CC	SVOC-8270-W-	ICV	/5975.I\sh122821	12/28/2021 9:19:	1	R372497		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14955044	28-Dec-21_CCV	SVOC-8270-W-	ICV	/5975.I\sh122821\	12/28/2021 9:19:	1	R372497		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	2.28179	2.28179		2	0	0	0.0206	0.1	10	114%	80	120	0%	
2-Methylnaphthalene	A	ug/L	2.10954	2.10954		2	0	0	0.0176	0.1	10	105%	80	120	0%	
Acenaphthene	A	ug/L	2.36763	2.36763		2	0	0	0.0317	0.1	10	118%	80	120	0%	
Acenaphthylene	A	ug/L	2.25828	2.25828		2	0	0	0.025	0.1	10	113%	80	120	0%	
Anthracene	A	ug/L	2.34155	2.34155		2	0	0	0.0283	0.1	10	117%	80	120	0%	
Benzo(a)anthracene	A	ug/L	2.30648	2.30648		2	0	0	0.0272	0.1	10	115%	80	120	0%	
Benzo(a)pyrene	A	ug/L	2.2645	2.2645		2	0	0	0.0347	0.1	10	113%	80	120	0%	
Benzo(b)fluoranthene	A	ug/L	2.23296	2.23296		2	0	0	0.0226	0.1	10	112%	80	120	0%	
Benzo(g,h,i)perylene	A	ug/L	2.3215	2.3215		2	0	0	0.0267	0.1	10	116%	80	120	0%	
Benzo(k)fluoranthene	A	ug/L	2.19575	2.19575		2	0	0	0.0295	0.1	10	110%	80	120	0%	
Chrysene	A	ug/L	2.34022	2.34022		2	0	0	0.0458	0.1	10	117%	80	120	0%	
Dibenzo(a,h)anthracene	A	ug/L	2.26205	2.26205		2	0	0	0.0367	0.1	10	113%	80	120	0%	
Fluoranthene	A	ug/L	2.2695	2.2695		2	0	0	0.0233	0.1	10	113%	80	120	0%	
Fluorene	A	ug/L	2.39799	2.39799		2	0	0	0.0225	0.1	10	120%	80	120	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	2.26864	2.26864		2	0	0	0.0491	0.1	10	113%	80	120	0%	
Naphthalene	A	ug/L	2.05863	2.05863		2	0	0	0.029	0.1	10	103%	80	120	0%	
Phenanthrene	A	ug/L	2.35989	2.35989		2	0	0	0.0295	0.1	10	118%	80	120	0%	
Pyrene	A	ug/L	2.01204	2.01204		2	0	0	0.0239	0.1	10	101%	80	120	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
2-Fluorobiphenyl	S	ug/L	2.26258	2.26258		2	0	0	0.0444	0.1	10	113%	80	120	0%	
Nitrobenzene-d5	S	ug/L	2.38774	2.38774		2	0	0	0.0523	0.1	10	119%	80	120	0%	
Terphenyl-d14	S	ug/L	1.939	1.939		2	0	0	0.0563	0.1	10	97%	80	120	0%	
o-Terphenyl	X	ug/L	2.22841	2.22841		2	0	0	0.0654	0.1	10	111%	80	120	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14955045	28-Dec-21_ISTB	SVOC-8270-W-	SAMP	/5975.I\sh122821\	12/28/2021 9:51:	1	R372497		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14955045	28-Dec-21_ISTB	SVOC-8270-W-	SAMP	75975.I\sh122821	12/28/2021 9:51:	1	R372497		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0206	0.1	10	0%	0	0	0%	
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0176	0.1	10	0%	0	0	0%	
Acenaphthene	A	ug/L	0	0		0	0	0	0.0317	0.1	10	0%	0	0	0%	
Acenaphthylene	A	ug/L	0	0		0	0	0	0.025	0.1	10	0%	0	0	0%	
Anthracene	A	ug/L	0	0		0	0	0	0.0283	0.1	10	0%	0	0	0%	
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.0272	0.1	10	0%	0	0	0%	
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.0347	0.1	10	0%	0	0	0%	
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.0226	0.1	10	0%	0	0	0%	
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.0267	0.1	10	0%	0	0	0%	
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.0295	0.1	10	0%	0	0	0%	
Chrysene	A	ug/L	0	0		0	0	0	0.0458	0.1	10	0%	0	0	0%	
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.0367	0.1	10	0%	0	0	0%	
Fluoranthene	A	ug/L	0	0		0	0	0	0.0233	0.1	10	0%	0	0	0%	
Fluorene	A	ug/L	0	0		0	0	0	0.0225	0.1	10	0%	0	0	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.0491	0.1	10	0%	0	0	0%	
Naphthalene	A	ug/L	0	0		0	0	0	0.029	0.1	10	0%	0	0	0%	
Phenanthrene	A	ug/L	0	0		0	0	0	0.0295	0.1	10	0%	0	0	0%	
Pyrene	A	ug/L	0	0		0	0	0	0.0239	0.1	10	0%	0	0	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
2-Fluorobiphenyl	S	ug/L	0	0		5	0	0	0.0444	0.1	10	0%	25	94	0%	S
Nitrobenzene-d5	S	ug/L	0	0		5	0	0	0.0523	0.1	10	0%	19	102	0%	S
Terphenyl-d14	S	ug/L	0	0		5	0	0	0.0563	0.1	10	0%	39	106	0%	S
o-Terphenyl	X	ug/L	0	0		200	0	0	0.0654	0.1	10	0%	40	140	0%	S

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14955048	MB-162432	SVOC-8270-W-	MBLK	75975.I\sh122821	12/28/2021 10:2	1	162432	12/22/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14955048	MB-162432	SVOC-8270-W-	MBLK	/5975.I\sh122821\	12/28/2021 10:2	1	162432	12/22/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0206	0.05	10	0%				0%
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0176	0.05	10	0%				0%
Naphthalene	A	ug/L	0	0		0	0	0	0.029	0.05	10	0%				0%
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14955049	MB-162432	SVOC-8270-W-	MBLK	/5975.I\sh122821\	12/28/2021 10:5	20	162432	12/22/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
2-Fluorobiphenyl	S	ug/L	3.35437	67.0874		100	0	0	0.888	2	10	67%	53	106		0%
Nitrobenzene-d5	S	ug/L	3.719	74.38		100	0	0	1.046	2	10	74%	55	111		0%
Terphenyl-d14	S	ug/L	4.89714	97.9428		100	0	0	1.126	2	10	98%	58	132		0%
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14955050	LLCS-162432	SVOC-8270-W-	LCS-DOD	/5975.I\sh122821\	12/28/2021 11:2	1	162432	12/22/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	3.02653	3.02653		5	0	0	0.0206	0.1	10	61%	41	115		0%
2-Methylnaphthalene	A	ug/L	2.69949	2.69949		5	0	0	0.0176	0.1	10	54%	39	114		0%
Naphthalene	A	ug/L	2.56287	2.56287		5	0	0	0.029	0.1	10	51%	43	114		0%
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14955051	LLCS-162432	SVOC-8270-W-	LCS-DOD	/5975.I\sh122821\	12/29/2021 12:0	20	162432	12/22/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
2-Fluorobiphenyl	S	ug/L	2.71144	54.2288		100	0	0	0.888	2	10	54%	53	106		0%
Nitrobenzene-d5	S	ug/L	3.1359	62.718		100	0	0	1.046	2	10	63%	55	111		0%
Terphenyl-d14	S	ug/L	5.58659	111.7318		100	0	0	1.126	2	10	112%	58	132		0%
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14955052	LLCSD-162432	SVOC-8270-W-	LCSD-DOD	/5975.I\sh122821\	12/29/2021 12:3	1	162432	12/22/2021	0	1E+07						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14955052	LLCSD-162432	SVOC-8270-W-	LCSD-DOD	/5975.I\sh122821\	12/29/2021 12:3	1	162432	12/22/2021	0	1E+07						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	2.45464	2.45464		5	0	3.02653	0.0206	0.1	10	49%	41	115	21%	
2-Methylnaphthalene	A	ug/L	2.19556	2.19556		5	0	2.69949	0.0176	0.1	10	44%	39	114	21%	
Naphthalene	A	ug/L	2.03253	2.03253		5	0	2.56287	0.029	0.1	10	41%	43	114	23%	S
2-Fluorobiphenyl	S	ug/L	4.29935	4.29935		5	0	0	0.0444	0.1	10	86%	53	106	0%	
Nitrobenzene-d5	S	ug/L	5.35939	5.35939		5	0	0	0.0523	0.1	10	107%	55	111	0%	
Terphenyl-d14	S	ug/L	6.65255	6.65255		5	0	0	0.0563	0.1	10	133%	58	132	0%	S
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14955053	B21121613-002	SVOC-8270-W-	SAMP	/5975.I\sh122821\	12/29/2021 1:07:	1	162392	12/21/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0200026	0.1	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0170896	0.1	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.028159	0.1	10	0%	0	0	0%	U
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14955054	B21121613-002	SVOC-8270-W-	SAMP	/5975.I\sh122821\	12/29/2021 1:39:	20	162392	12/21/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
2-Fluorobiphenyl	S	ug/L	2.73816	53.1750672		97.1	0	0	0.862248	1.942	10	55%	53	106	0%	
Nitrobenzene-d5	S	ug/L	2.21972	43.1069624		97.1	0	0	1.015666	1.942	10	44%	55	111	0%	S
Terphenyl-d14	S	ug/L	4.63288	89.9705296		97.1	0	0	1.093346	1.942	10	93%	58	132	0%	
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14955055	B21121616-001	SVOC-8270-W-	SAMP	/5975.I\sh122821\	12/29/2021 2:12:	1	162392	12/21/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	2.20751	2.2295851		0	0	0	0.020806	0.101	10	0%	0	0	0%	
2-Methylnaphthalene	A	ug/L	0.95101	0.9605201		0	0	0	0.017776	0.101	10	0%	0	0	0%	
Naphthalene	A	ug/L	4.81048	4.8585848		0	0	0	0.02929	0.101	10	0%	0	0	0%	
2-Fluorobiphenyl	S	ug/L	2.43619	2.4605519		5.05	0	0	0.044844	0.101	10	49%	53	106	0%	S
Nitrobenzene-d5	S	ug/L	2.12627	2.1475327		5.05	0	0	0.052823	0.101	10	43%	55	111	0%	S
Terphenyl-d14	S	ug/L	4.06718	4.1078518		5.05	0	0	0.056863	0.101	10	81%	58	132	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14955056	B21121622-001	SVOC-8270-W-	SAMP	/5975.I\sh122821\	12/29/2021 2:45:	1	162392	12/21/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0196112	0.1	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0167552	0.1	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.027608	0.1	10	0%	0	0	0%	U
2-Fluorobiphenyl	S	ug/L	3.14768	2.99659136		4.76	0	0	0.0422688	0.1	10	63%	53	106	0%	
Nitrobenzene-d5	S	ug/L	3.76231	3.58171912		4.76	0	0	0.0497896	0.1	10	75%	55	111	0%	
Terphenyl-d14	S	ug/L	3.91529	3.72735608		4.76	0	0	0.0535976	0.1	10	78%	58	132	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14955057	B21121622-002	SVOC-8270-W-	SAMP	/5975.I\sh122821\	12/29/2021 3:17:	1	162392	12/21/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0196112	0.1	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0167552	0.1	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.027608	0.1	10	0%	0	0	0%	U
2-Fluorobiphenyl	S	ug/L	3.24773	3.09183896		4.76	0	0	0.0422688	0.1	10	65%	53	106	0%	
Nitrobenzene-d5	S	ug/L	3.64216	3.46733632		4.76	0	0	0.0497896	0.1	10	73%	55	111	0%	
Terphenyl-d14	S	ug/L	4.65043	4.42720936		4.76	0	0	0.0535976	0.1	10	93%	58	132	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14955058	B21121622-003	SVOC-8270-W-	SAMP	/5975.I\sh122821\	12/29/2021 3:50:	1	162392	12/21/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.021836	0.106	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.018656	0.106	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.03074	0.106	10	0%	0	0	0%	U

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14955059	B21121622-003	SVOC-8270-W-	SAMP	/5975.I\sh122821\	12/29/2021 4:23:	20	162392	12/21/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
2-Fluorobiphenyl	S	ug/L	2.24548	47.604176		106	0	0	0.94128	2.12	10	45%	53	106	0%	S
Nitrobenzene-d5	S	ug/L	3.42778	72.668936		106	0	0	1.10876	2.12	10	69%	55	111	0%	
Terphenyl-d14	S	ug/L	5.03885	106.82362		106	0	0	1.19356	2.12	10	101%	58	132	0%	



Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14955060	B21121623-001	SVOC-8270-W-	SAMP	/5975.I\sh122821\	12/29/2021 4:55:	1	162392	12/21/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0196112	0.1	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0167552	0.1	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.027608	0.1	10	0%	0	0	0%	U
2-Fluorobiphenyl	S	ug/L	3.28379	3.12616808		4.76	0	0	0.0422688	0.1	10	66%	53	106	0%	
Nitrobenzene-d5	S	ug/L	3.62325	3.449334		4.76	0	0	0.0497896	0.1	10	72%	55	111	0%	
Terphenyl-d14	S	ug/L	5.0373	4.7955096		4.76	0	0	0.0535976	0.1	10	101%	58	132	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14955061	28-Dec-21_CC	SVOC-8270-W-	CCV	/5975.I\sh122821\	12/29/2021 5:28:	1	R372497		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	2.05854	2.05854		2	0	0	0.0206	0.1	10	103%	50	150	0%	
2-Methylnaphthalene	A	ug/L	1.80326	1.80326		2	0	0	0.0176	0.1	10	90%	50	150	0%	
Naphthalene	A	ug/L	1.56861	1.56861		2	0	0	0.029	0.1	10	78%	50	150	0%	
2-Fluorobiphenyl	S	ug/L	1.70703	1.70703		2	0	0	0.0444	0.1	10	85%	50	150	0%	
Nitrobenzene-d5	S	ug/L	2.10871	2.10871		2	0	0	0.0523	0.1	10	105%	50	150	0%	
Terphenyl-d14	S	ug/L	1.84995	1.84995		2	0	0	0.0563	0.1	10	92%	50	150	0%	

File Name	Sample Name	Line No.	Test Code	Multiplier	Divisor	Method Name
Dec2801.d	28-Dec-21_TUNE_1	1		1	1	5975Tune.M
Dec2802.d	28-Dec-21_CAL_7	2	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Dec2803.d	28-Dec-21_CAL_6	3	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Dec2804.d	28-Dec-21_CAL_5	4	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Dec2805.d	28-Dec-21_CAL_4	5	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Dec2806.d	28-Dec-21_CAL_3	6	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Dec2807.d	28-Dec-21_CAL_2	7	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Dec2808.d	28-Dec-21_CAL_1	8	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Dec2809.d	28-Dec-21_CCV_9	9	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Dec2810.d	28-Dec-21_ISTBLK_10	10	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Dec2811.d	MB-162432	11	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Dec2812.d	MB-162432	12	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Dec2813.d	LLCS-162432	13	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Dec2814.d	LLCS-162432	14	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Dec2815.d	LLCSD-162432	15	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Dec2816.d	B21121613-002A	16	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Dec2817.d	B21121613-002A	17	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Dec2818.d	B21121616-001B	18	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Dec2819.d	B21121622-001A	19	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Dec2820.d	B21121622-002A	20	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Dec2821.d	B21121622-003A	21	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Dec2822.d	B21121622-003A	22	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Dec2823.d	B21121623-001B	23	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Dec2824.d	28-Dec-21_CCV_24	24	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Dec2825.d	28-Dec-21_TUNE_25	25		1	1	5975Tune.M
Dec2826.d	28-Dec-21_CCV_26	26	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Dec2827.d	28-Dec-21_ISTBLK_27	27	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Dec2828.d	B21121841-001A	28	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Dec2829.d	B21121841-001A	29	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Dec2830.d	B21121841-001ALMS	30	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Dec2831.d	B21121841-002A	31	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Dec2832.d	B21121841-002A	32	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Dec2833.d	B21121841-003A	33	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Dec2834.d	B21121841-003A	34	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Dec2835.d	B21121841-004A	35	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Dec2836.d	B21121841-004A	36	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Dec2837.d	28-Dec-21_CCV_37	26	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M









Tune Evaluation Report

Data Path: \\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2801.D
 Acq on: 12/28/2021 5:06:43 PM
 Operator: LIMS import
 Sample: 28-Dec-21_TUNE_1
 Inst Name: GCMS
 ALS Vial: 1
 Method: \\MASSHUNTER\Org\Data\SV5975.I\Methods\DFTPP5975625.m




Target Mass	Rel. To Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Pass/Fail
51	198	30	60	50.7	175808	Pass
68	69	0	2	0.0	0	Pass
70	69	0	2	0.5	1441	Pass
127	198	40	60	49.1	170304	Pass
197	198	0	1	0.0	0	Pass
198	198	100	100	100.0	347072	Pass
199	198	5	9	6.6	22904	Pass
275	198	10	30	29.6	102792	Pass
365	198	1	100	2.9	10127	Pass
441	443	1E-10	150	98.7	34384	Pass
442	198	40	100	50.7	176128	Pass
443	442	17	23	19.8	34832	Pass
69	69	100	100	100.0	275072	Pass

Tune Evaluation Report

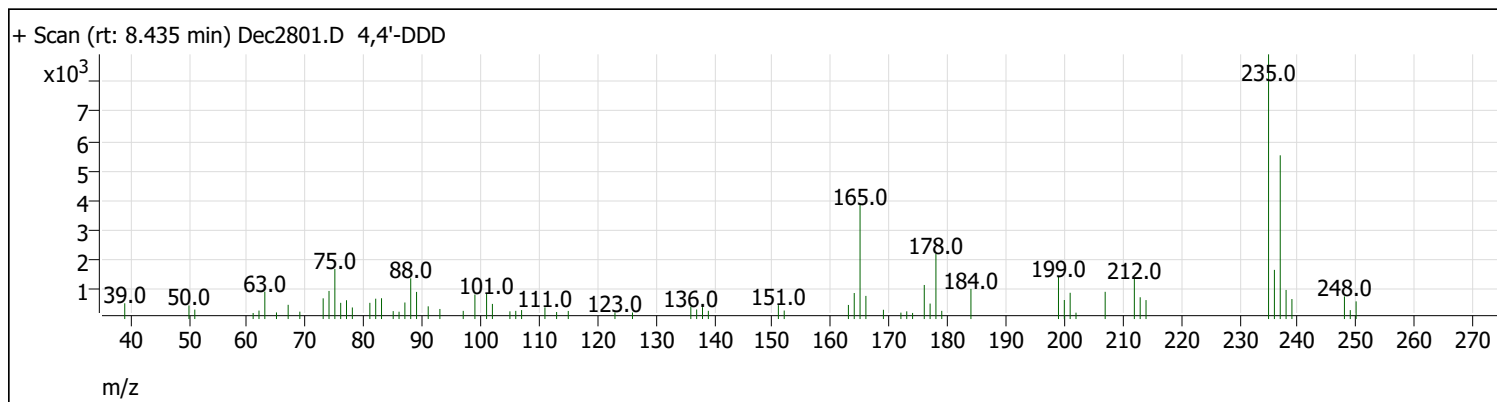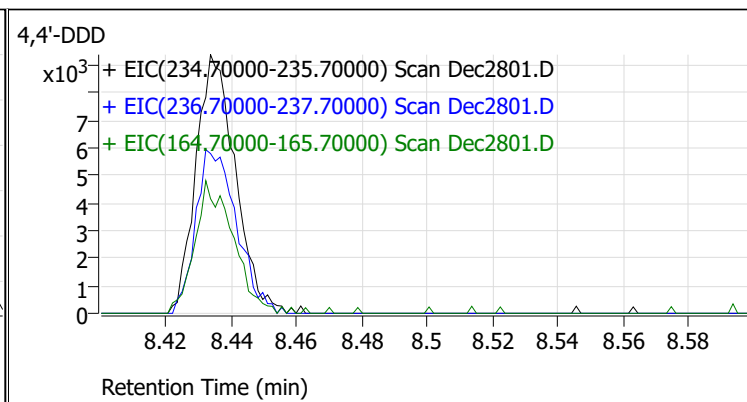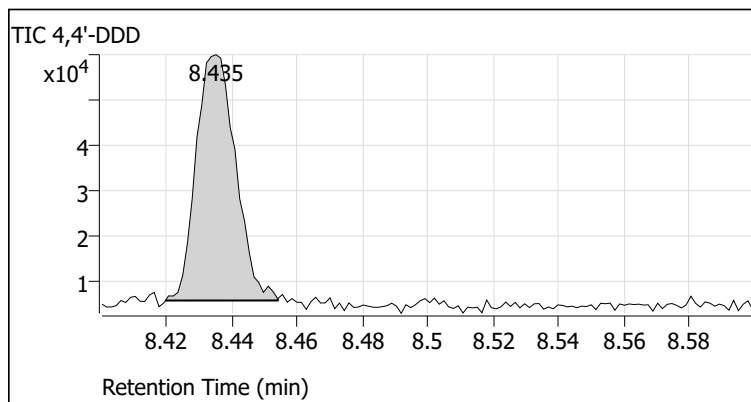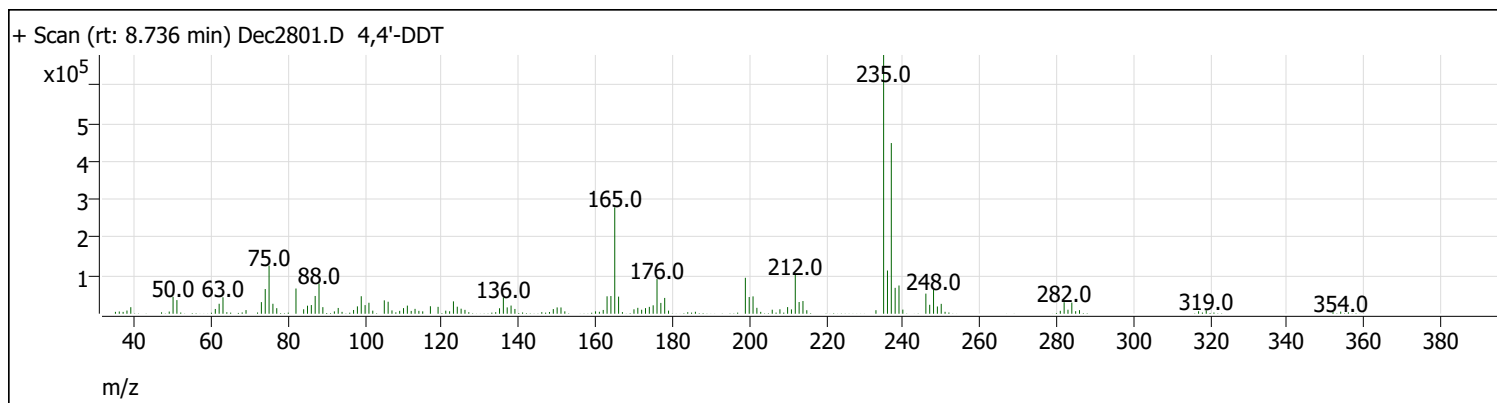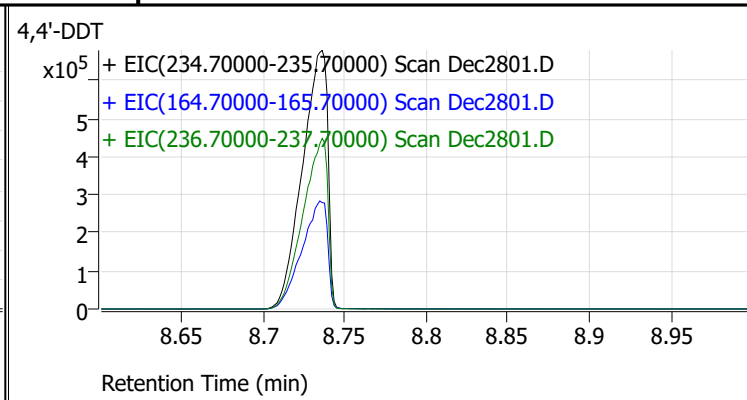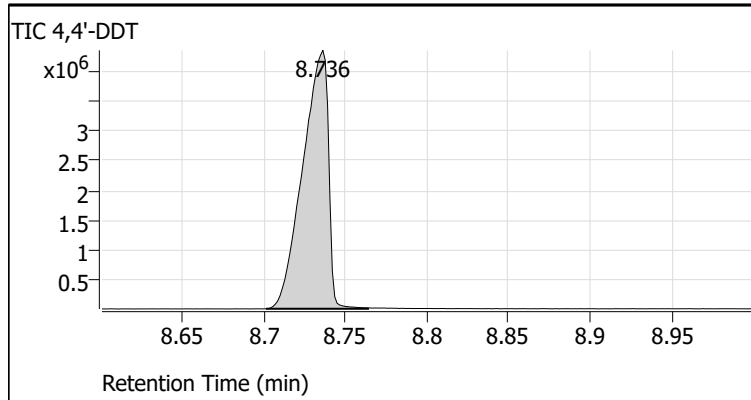

Tune Evaluation Report


+ Scan (rt: 8.181-8.220 min, 28 scans) Dec2801.D 4,4'-DDE

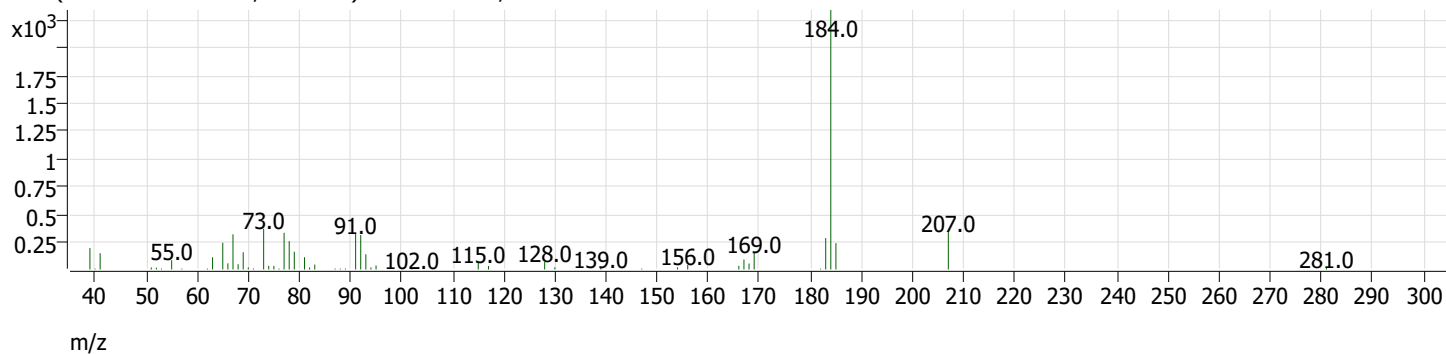


Compound Name	Expected RT	Observed RT	TIC Area	Breakdown %	Pass/Fail
4,4'-DDT	8.800	8.736	4761627	0.9	Pass
4,4'-DDD	8.500	8.435	45444		
4,4'-DDE	8.200	0.000	0		

Tune Evaluation Report

+ Scan (rt: 6.431 min) Dec2801.D Pentachlorophenol



+ Scan (rt: 7.965 min) Dec2801.D Benzidine




Compound Name	Expected RT	Observed RT	Tailing Factor	PGF	Pass/Fail
Pentachlorophenol	6.800	6.431	0.4	25.5	Pass
Benzidine	8.400	7.965	0.3	16.6	Pass

Calibration Report

Batch Path	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\QuantResults\122821 bna SIM 1.batch.bin	Analyst Name	BL2000\jheine
Analysis Time	12/29/2021 9:21 AM	Reporter Name	BL2000\jheine
Report Time	1/6/2022 12:26:33 PM	Batch State	Processed
Last Calib Update	12/29/2021 8:56 AM	Quant Report Version	10.0
Quant Batch Version	10.0		

Nitrobenzene-d5 %RSE =

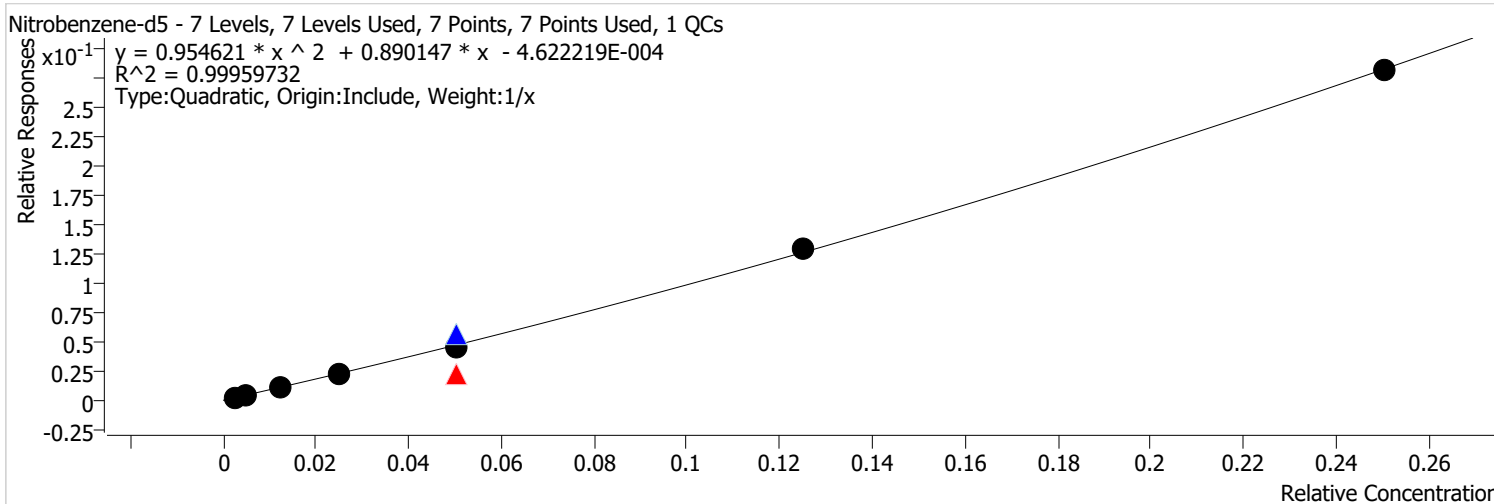


Calibration STD Path	Cal Type	Level	Enabled	Resp.	Exp. Conc	Resp. Factor	Level RSD
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2808.D	Calibration	1	x	515	0.1000	0.7107	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2807.D	Calibration	2	x	1083	0.2000	0.8020	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2806.D	Calibration	3	x	3113	0.5000	0.9012	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2805.D	Calibration	4	x	6936	1.0000	0.8751	
\\MASSHUNTER\Org\Data\SV5975.I\sh122021\1 e8270d bna SIM\Dec2025.D	CC	CCV	x	9501	2.0000	0.4341	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2809.D	QC	ICV	x	18569	2.0000	1.1215	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2804.D	Calibration	5	x	14443	2.0000	0.8897	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2803.D	Calibration	6	x	42512	5.0000	1.0311	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2802.D	Calibration	7	x	92065	10.0000	1.1223	

Calibration Report

Batch Path	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\QuantResults\122821 bna SIM 1.batch.bin	Analyst Name	BL2000\jheine
Analysis Time	12/29/2021 9:21 AM	Reporter Name	BL2000\jheine
Report Time	1/6/2022 12:26:38 PM	Batch State	Processed
Last Calib Update	12/29/2021 8:56 AM	Quant Report Version	10.0
Quant Batch Version	10.0		

Naphthalene %RSE = 4.7




Calibration STD Path	Cal Type	Level	Enabled	Resp.	Exp. Conc	Resp. Factor	Level RSD
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2808.D	Calibration	1	x	2075	0.1000	1.4471	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2807.D	Calibration	2	x	3569	0.2000	1.3069	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2806.D	Calibration	3	x	9084	0.5000	1.3362	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2805.D	Calibration	4	x	19154	1.0000	1.3309	
\\MASSHUNTER\Org\Data\SV5975.I\sh122021\1 e8270d bna SIM\Dec2025.D	CC	CCV	x	47467	2.0000	1.3267	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2809.D	QC	ICV	x	44031	2.0000	1.3825	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2804.D	Calibration	5	x	37909	2.0000	1.2781	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2803.D	Calibration	6	x	98629	5.0000	1.2899	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2802.D	Calibration	7	x	199178	10.0000	1.4130	

Calibration Report

Batch Path	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\QuantResults\122821 bna SIM 1.batch.bin	Analyst Name	BL2000\jheine
Analysis Time	12/29/2021 9:21 AM	Reporter Name	BL2000\jheine
Report Time	1/6/2022 12:26:38 PM	Batch State	Processed
Last Calib Update	12/29/2021 8:56 AM	Quant Report Version	10.0
Quant Batch Version	10.0		

2-Methylnaphthalene %RSE = 5.7

2-Methylnaphthalene - 7 Levels, 7 Levels Used, 7 Points, 7 Points Used, 1 QCs




Calibration STD Path	Cal Type	Level	Enabled	Resp.	Exp. Conc	Resp. Factor	Level RSD
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2808.D	Calibration	1	x	1176	0.1000	0.8203	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2807.D	Calibration	2	x	2170	0.2000	0.7946	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2806.D	Calibration	3	x	5515	0.5000	0.8112	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2805.D	Calibration	4	x	10932	1.0000	0.7596	
\\MASSHUNTER\Org\Data\SV5975.I\sh122021\1 e8270d bna SIM\Dec2025.D	CC	CCV	x	27745	2.0000	0.7755	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2809.D	QC	ICV	x	26021	2.0000	0.8170	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2804.D	Calibration	5	x	21520	2.0000	0.7255	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2803.D	Calibration	6	x	54126	5.0000	0.7079	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2802.D	Calibration	7	x	113224	10.0000	0.8032	

Calibration Report

Batch Path	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\QuantResults\122821 bna SIM 1.batch.bin	Analyst Name	BL2000\jheine
Analysis Time	12/29/2021 9:21 AM	Reporter Name	BL2000\jheine
Report Time	1/6/2022 12:26:38 PM	Batch State	Processed
Last Calib Update	12/29/2021 8:56 AM	Quant Report Version	10.0
Quant Batch Version	10.0		

1-Methylnaphthalene %RSE = 8.2




Calibration STD Path	Cal Type	Level	Enabled	Resp.	Exp. Conc	Resp. Factor	Level RSD
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2808.D	Calibration	1	x	1191	0.1000	0.8302	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2807.D	Calibration	2	x	2021	0.2000	0.7400	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2806.D	Calibration	3	x	4850	0.5000	0.7134	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2805.D	Calibration	4	x	9969	1.0000	0.6926	
\\MASSHUNTER\Org\Data\SV5975.I\sh122021\1 e8270d bna SIM\Dec2025.D	CC	CCV	x	25998	2.0000	0.7267	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2809.D	QC	ICV	x	26026	2.0000	0.8172	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2804.D	Calibration	5	x	19512	2.0000	0.6578	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2803.D	Calibration	6	x	50414	5.0000	0.6593	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2802.D	Calibration	7	x	101559	10.0000	0.7205	

Calibration Report

Batch Path	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\QuantResults\122821 bna SIM 1.batch.bin		
Analysis Time	12/29/2021 9:21 AM	Analyst Name	BL2000\jheine
Report Time	1/6/2022 12:26:38 PM	Reporter Name	BL2000\jheine
Last Calib Update	12/29/2021 8:56 AM	Batch State	Processed
Quant Batch Version	10.0	Quant Report Version	10.0

2-Fluorobiphenyl %RSE =

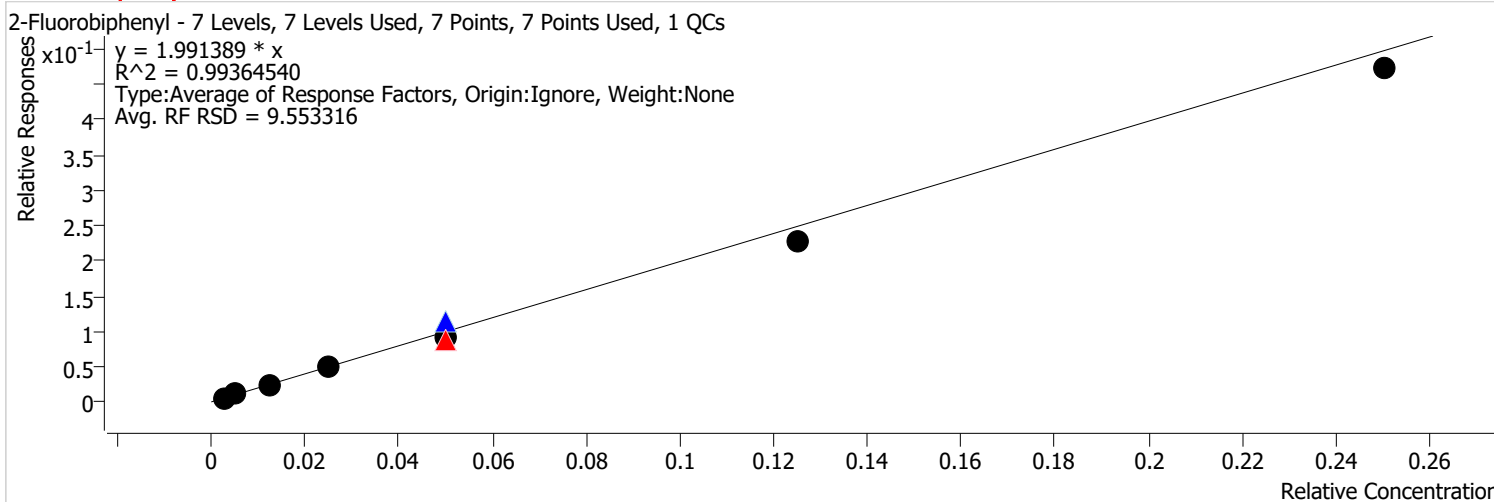


Calibration STD Path	Cal Type	Level	Enabled	Resp.	Exp. Conc	Resp. Factor	Level RSD
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2808.D	Calibration	1	x	1855	0.1000	2.3524	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2807.D	Calibration	2	x	3084	0.2000	2.1159	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2806.D	Calibration	3	x	7476	0.5000	1.9824	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2805.D	Calibration	4	x	15555	1.0000	1.9615	
\\MASSHUNTER\Org\Data\SV5975.I\sh122021\1 e8270d bna SIM\Dec2025.D	CC	CCV	x	41599	2.0000	1.7675	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2809.D	QC	ICV	x	38269	2.0000	2.2528	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2804.D	Calibration	5	x	30043	2.0000	1.8026	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2803.D	Calibration	6	x	77505	5.0000	1.8353	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2802.D	Calibration	7	x	160009	10.0000	1.8897	

Calibration Report

Batch Path	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\QuantResults\122821 bna SIM 1.batch.bin		
Analysis Time	12/29/2021 9:21 AM	Analyst Name	BL2000\jheine
Report Time	1/6/2022 12:26:38 PM	Reporter Name	BL2000\jheine
Last Calib Update	12/29/2021 8:56 AM	Batch State	Processed
Quant Batch Version	10.0	Quant Report Version	10.0

Terphenyl-d14 %RSE =

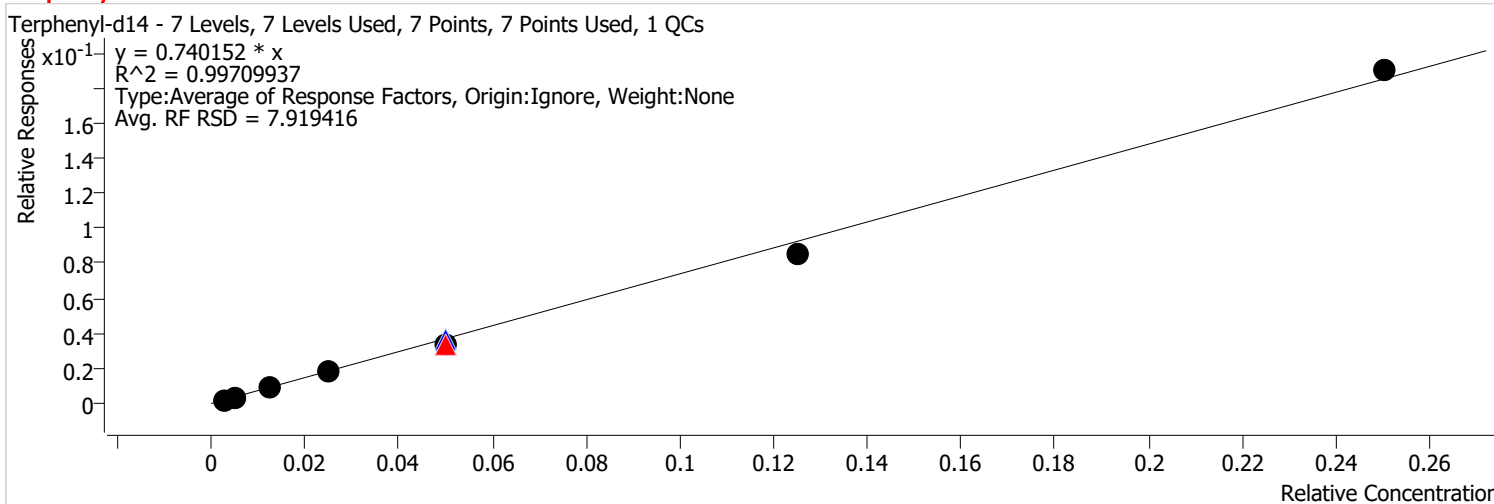

Calibration STD Path	Cal Type	Level	Enabled	Resp.	Exp. Conc	Resp. Factor	Level RSD
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2808.D	Calibration	1	x	1041	0.1000	0.8497	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2807.D	Calibration	2	x	1955	0.2000	0.7620	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2806.D	Calibration	3	x	4385	0.5000	0.7380	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2805.D	Calibration	4	x	9183	1.0000	0.7076	
\\MASSHUNTER\Org\Data\SV5975.I\sh122021\1 e8270d bna SIM\Dec2025.D	CC	CCV	x	22770	2.0000	0.6617	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2809.D	QC	ICV	x	21623	2.0000	0.7176	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2804.D	Calibration	5	x	18378	2.0000	0.6806	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2803.D	Calibration	6	x	48329	5.0000	0.6840	
\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2802.D	Calibration	7	x	102521	10.0000	0.7592	

Initial Calibration Report - GCMS

Method Path
 Method File
 Batch Name \\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\QuantResults\122821 bna SIM 1.batch.bin
 Last Calib Update 12/29/2021 8:56:55 AM

Level Name	Calibration Files	Acq. Date-Time	Level Last Update Time
7	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2802.D	12/28/2021 5:30:40 PM	12/29/2021 8:56:55 AM
6	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2803.D	12/28/2021 6:03:21 PM	12/29/2021 8:56:55 AM
5	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2804.D	12/28/2021 6:35:53 PM	12/29/2021 8:56:55 AM
4	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2805.D	12/28/2021 7:08:33 PM	12/29/2021 8:56:55 AM
3	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2806.D	12/28/2021 7:41:06 PM	12/29/2021 8:56:55 AM
2	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2807.D	12/28/2021 8:13:46 PM	12/29/2021 8:56:55 AM
1	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2808.D	12/28/2021 8:46:23 PM	12/29/2021 8:56:55 AM

Compound	Curve Fit	7	6	5	4	3	2	1	Avg RF	%RSD
I 1,4-Dichlorobenzene-d4										
S Nitrobenzene-d5	Quadratic	1.1223	1.0311	0.8897	0.8751	0.9012	0.8020	0.7107	0.9046	15.145
I Naphthalene-d8										
T Naphthalene	Avg RF	1.4130	1.2899	1.2781	1.3309	1.3362	1.3069	1.4471	1.3431	4.734
T 2-Methylnaphthalene	Avg RF	0.8032	0.7079	0.7255	0.7596	0.8112	0.7946	0.8203	0.7746	5.709
T 1-Methylnaphthalene	Avg RF	0.7205	0.6593	0.6578	0.6926	0.7134	0.7400	0.8302	0.7163	8.217
I Acenaphthene-d10										
S 2-Fluorobiphenyl	Avg RF	1.8897	1.8353	1.8026	1.9615	1.9824	2.1159	2.3524	1.9914	9.553
I Chrysene-d12										
S Terphenyl-d14	Avg RF	0.7592	0.6840	0.6806	0.7076	0.7380	0.7620	0.8497	0.7402	7.919

(RedFont and #) = Outlier Flag; (I) = Internal Standard; (T) = Target; (S) = Surrogate; (M) = Matrix Spike

Compounds with Curve fitting not using Avg Response Factor:

Compound	Curve Fit	Curve Fit Formula	Curve Fit R2
S Nitrobenzene-d5	Quadratic	$y = 0.954621 * x ^ 2 + 0.890147 * x - 4.622219E-004$	0.999597

(RedFont and #) = Outlier Flag; (I) = Internal Standard; (T) = Target; (S) = Surrogate; (M) = Matrix Spike

Quantitative Analysis Results Summary Report

Batch Path	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1_e8270c_bna_SIM\QuantResults\122821_bna_SIM_1.batch.bin	Analyst Name	BL2000\jheine
Analysis Time	12/29/2021 9:21 AM	Reporter Name	BL2000\jheine
Report Time	1/6/2022 12:28:37 PM	Batch State	Processed
Last Calib Update	12/29/2021 8:56 AM	Quant Report Version	10.0
Quant Batch Version	10.0		

Sequence Table

Data File	sample Name	Sample Type	Vial Position	Inj Vol	Level	Acq Method File
Dec2802.D	28-Dec-21_CAL_7	Cal	2	0.1	7	5975BNASIM
Dec2803.D	28-Dec-21_CAL_6	Cal	3	0.1	6	5975BNASIM
Dec2804.D	28-Dec-21_CAL_5	Cal	4	0.1	5	5975BNASIM
Dec2805.D	28-Dec-21_CAL_4	Cal	5	0.1	4	5975BNASIM
Dec2806.D	28-Dec-21_CAL_3	Cal	6	0.1	3	5975BNASIM
Dec2807.D	28-Dec-21_CAL_2	Cal	7	0.1	2	5975BNASIM
Dec2808.D	28-Dec-21_CAL_1	Cal	8	0.1	1	5975BNASIM
Dec2809.D	28-Dec-21_CCV_9	QC	9	0.1	ICV	5975BNASIM

Quantitation Results

Compound: Nitrobenzene-d5

Data File	Sample Type	ISTD	RT	Resp	ISTD Resp	Resp Ratio	Final Conc	Exp. Conc	Accuracy
Dec2802.D	Calibration	1,4-Dichlorobenzene-d4	5.180	92065	328131	0.2806	9.9659	10.0000	99.7
Dec2803.D	Calibration	1,4-Dichlorobenzene-d4	5.180	42512	329834	0.1289	5.1120	5.0000	102.2
Dec2804.D	Calibration	1,4-Dichlorobenzene-d4	5.193	14443	324694	0.0445	1.9208	2.0000	96.0
Dec2805.D	Calibration	1,4-Dichlorobenzene-d4	5.193	6936	317026	0.0219	0.9782	1.0000	97.8
Dec2806.D	Calibration	1,4-Dichlorobenzene-d4	5.193	3113	276368	0.0113	0.5197	0.5000	103.9
Dec2807.D	Calibration	1,4-Dichlorobenzene-d4	5.205	1083	269989	0.0040	0.1999	0.2000	99.9
Dec2808.D	Calibration	1,4-Dichlorobenzene-d4	5.205	515	289704	0.0018	0.1003	0.1000	100.3
Dec2809.D	QC	1,4-Dichlorobenzene-d4	5.181	18569	331151	0.0561	2.3877	2.0000	119.4

Compound: Naphthalene

Data File	Sample Type	ISTD	RT	Resp	ISTD Resp	Resp Ratio	Final Conc	Exp. Conc	Accuracy
Dec2802.D	Calibration	Naphthalene-d8	5.990	199178	563856	0.3532	10.5198	10.0000	105.2
Dec2803.D	Calibration	Naphthalene-d8	5.991	98629	611694	0.1612	4.8018	5.0000	96.0
Dec2804.D	Calibration	Naphthalene-d8	5.991	37909	593232	0.0639	1.9031	2.0000	95.2
Dec2805.D	Calibration	Naphthalene-d8	5.991	19154	575703	0.0333	0.9908	1.0000	99.1
Dec2806.D	Calibration	Naphthalene-d8	5.991	9084	543848	0.0167	0.4974	0.5000	99.5
Dec2807.D	Calibration	Naphthalene-d8	5.991	3569	546111	0.0065	0.1946	0.2000	97.3
Dec2808.D	Calibration	Naphthalene-d8	5.991	2075	573640	0.0036	0.1077	0.1000	107.7
Dec2809.D	QC	Naphthalene-d8	5.991	44031	636971	0.0691	2.0586	2.0000	102.9

Compound: 2-Methylnaphthalene

Data File	Sample Type	ISTD	RT	Resp	ISTD Resp	Resp Ratio	Final Conc	Exp. Conc	Accuracy
Dec2802.D	Calibration	Naphthalene-d8	6.815	113224	563856	0.2008	10.3692	10.0000	103.7
Dec2803.D	Calibration	Naphthalene-d8	6.815	54126	611694	0.0885	4.5693	5.0000	91.4
Dec2804.D	Calibration	Naphthalene-d8	6.815	21520	593232	0.0363	1.8732	2.0000	93.7

Quantitative Analysis Results Summary Report

Compound: 2-Methylnaphthalene

Data File	Sample Type	ISTD	RT	Resp	ISTD Resp	Resp Ratio	Final Conc	Exp. Conc	Accuracy
Dec2805.D	Calibration	Naphthalene-d8	6.815	10932	575703	0.0190	0.9806	1.0000	98.1
Dec2806.D	Calibration	Naphthalene-d8	6.815	5515	543848	0.0101	0.5236	0.5000	104.7
Dec2807.D	Calibration	Naphthalene-d8	6.815	2170	546111	0.0040	0.2052	0.2000	102.6
Dec2808.D	Calibration	Naphthalene-d8	6.815	1176	573640	0.0021	0.1059	0.1000	105.9
Dec2809.D	QC	Naphthalene-d8	6.815	26021	636971	0.0409	2.1095	2.0000	105.5

Compound: 1-Methylnaphthalene

Data File	Sample Type	ISTD	RT	Resp	ISTD Resp	Resp Ratio	Final Conc	Exp. Conc	Accuracy
Dec2802.D	Calibration	Naphthalene-d8	6.927	101559	563856	0.1801	10.0587	10.0000	100.6
Dec2803.D	Calibration	Naphthalene-d8	6.927	50414	611694	0.0824	4.6027	5.0000	92.1
Dec2804.D	Calibration	Naphthalene-d8	6.927	19512	593232	0.0329	1.8368	2.0000	91.8
Dec2805.D	Calibration	Naphthalene-d8	6.927	9969	575703	0.0173	0.9670	1.0000	96.7
Dec2806.D	Calibration	Naphthalene-d8	6.927	4850	543848	0.0089	0.4980	0.5000	99.6
Dec2807.D	Calibration	Naphthalene-d8	6.927	2021	546111	0.0037	0.2066	0.2000	103.3
Dec2808.D	Calibration	Naphthalene-d8	6.927	1191	573640	0.0021	0.1159	0.1000	115.9
Dec2809.D	QC	Naphthalene-d8	6.915	26026	636971	0.0409	2.2818	2.0000	114.1

Compound: 2-Fluorobiphenyl

Data File	Sample Type	ISTD	RT	Resp	ISTD Resp	Resp Ratio	Final Conc	Exp. Conc	Accuracy
Dec2802.D	Calibration	Acenaphthene-d10	7.277	160009	338694	0.4724	9.4894	10.0000	94.9
Dec2803.D	Calibration	Acenaphthene-d10	7.277	77505	337847	0.2294	4.6080	5.0000	92.2
Dec2804.D	Calibration	Acenaphthene-d10	7.277	30043	333337	0.0901	1.8104	2.0000	90.5
Dec2805.D	Calibration	Acenaphthene-d10	7.277	15555	317203	0.0490	0.9850	1.0000	98.5
Dec2806.D	Calibration	Acenaphthene-d10	7.277	7476	301716	0.0248	0.4977	0.5000	99.5
Dec2807.D	Calibration	Acenaphthene-d10	7.277	3084	291537	0.0106	0.2125	0.2000	106.3
Dec2808.D	Calibration	Acenaphthene-d10	7.277	1855	315361	0.0059	0.1181	0.1000	118.1
Dec2809.D	QC	Acenaphthene-d10	7.277	38269	339738	0.1126	2.2626	2.0000	113.1


Compound: Terphenyl-d14

Data File	Sample Type	ISTD	RT	Resp	ISTD Resp	Resp Ratio	Final Conc	Exp. Conc	Accuracy
Dec2802.D	Calibration	Chrysene-d12	12.300	102521	540119	0.1898	10.2580	10.0000	102.6
Dec2803.D	Calibration	Chrysene-d12	12.300	48329	565286	0.0855	4.6204	5.0000	92.4
Dec2804.D	Calibration	Chrysene-d12	12.300	18378	540068	0.0340	1.8390	2.0000	92.0
Dec2805.D	Calibration	Chrysene-d12	12.300	9183	519103	0.0177	0.9560	1.0000	95.6
Dec2806.D	Calibration	Chrysene-d12	12.300	4385	475304	0.0092	0.4985	0.5000	99.7
Dec2807.D	Calibration	Chrysene-d12	12.300	1955	513253	0.0038	0.2059	0.2000	103.0
Dec2808.D	Calibration	Chrysene-d12	12.300	1041	490023	0.0021	0.1148	0.1000	114.8
Dec2809.D	QC	Chrysene-d12	12.288	21623	602674	0.0359	1.9390	2.0000	97.0

Quantitation Results Report (QT Reviewed)

Data File	Dec2802.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	12/28/2021 5:30:40 PM
Sample Name	28-Dec-21_CAL_7	Instrument	GCMS
Vial	2	Multiplier	1.00
DA Method File		Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	122821 bna SIM 1.batch.bin	Last Calib Update	12/29/2021 8:56:55 AM

Ref Library

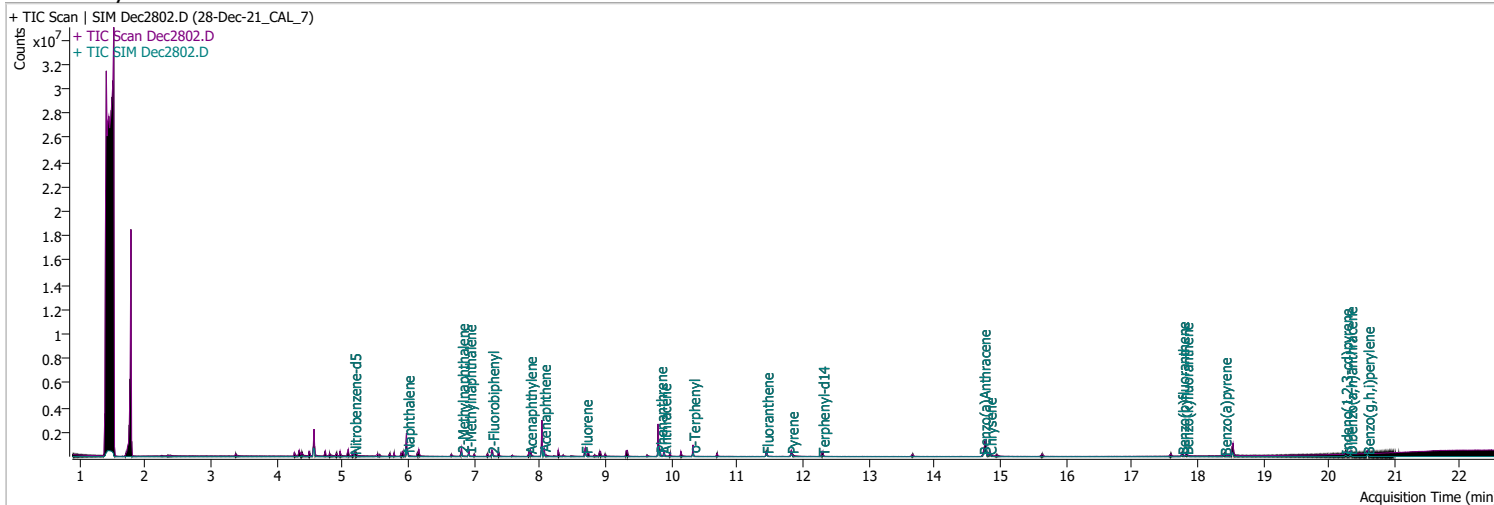

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
----------	----	------	-------	-------	-------	----------

Internal Standards

System Monitoring Compounds

S Nitrobenzene-d5	5.180	82.0	92065	9.9659	ng/ml	m	-0.013
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 199.32%		*	
S 2-Fluorobiphenyl	7.277	172.0	160009	9.4894	ng/ml		0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 189.79%		*	
S Terphenyl-d14	12.300	244.0	102521	10.2580	ng/ml		0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 205.16%		*	




Target Compounds

Compound	RT	QIon	Resp.	Conc.	Units	QValue
T Naphthalene	5.990	128.0	199178	10.5198	ng/ml	99
T 2-Methylnaphthalene	6.815	141.0	113224	10.3692	ng/ml	98
T 1-Methylnaphthalene	6.927	141.0	101559	10.0587	ng/ml	99




(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	9.9659	5.18	-0.01	92065 (m)	54.0	32.9	21.6	40.2
					128.0	26.1	21.3	39.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	10.5198	5.99	0.00	199178	102.0	14.8	0.0	46.6
					129.0	11.2	7.6	14.1

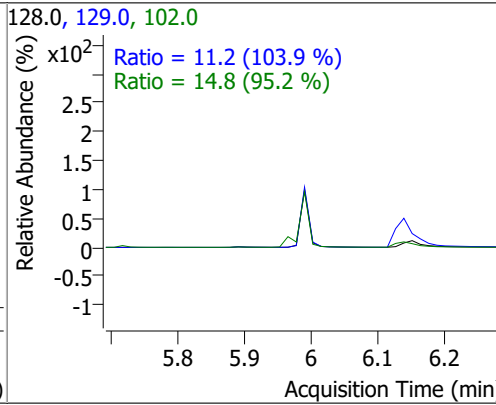


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	10.3692	6.81	0.00	113224	142.0	150.6	103.3	191.8
					115.0	52.5	36.8	68.3




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	10.0587	6.93	0.00	101559	142.0	112.6	77.9	144.7
					115.0	62.1	44.4	82.5

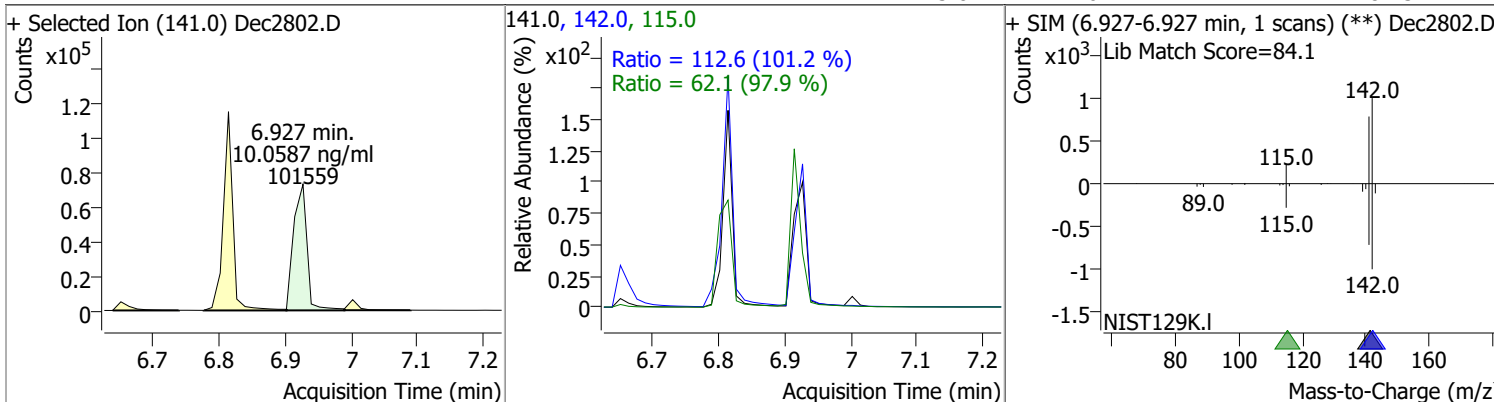

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	9.4894	7.28	0.00	160009	171.0	38.0	26.4	49.0

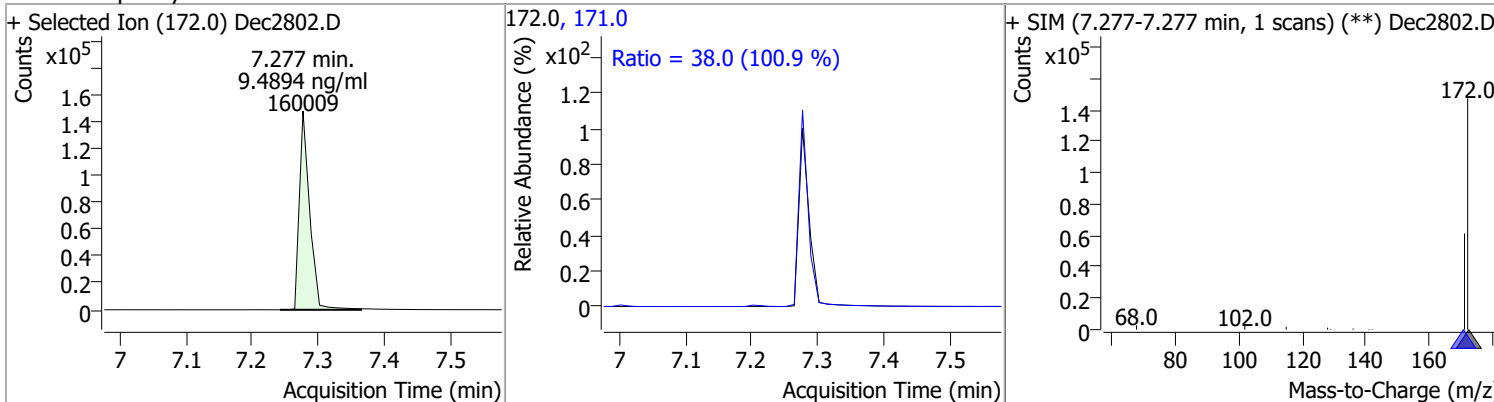


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	10.2580	12.30	0.00	102521	122.0	14.3	9.6	17.9

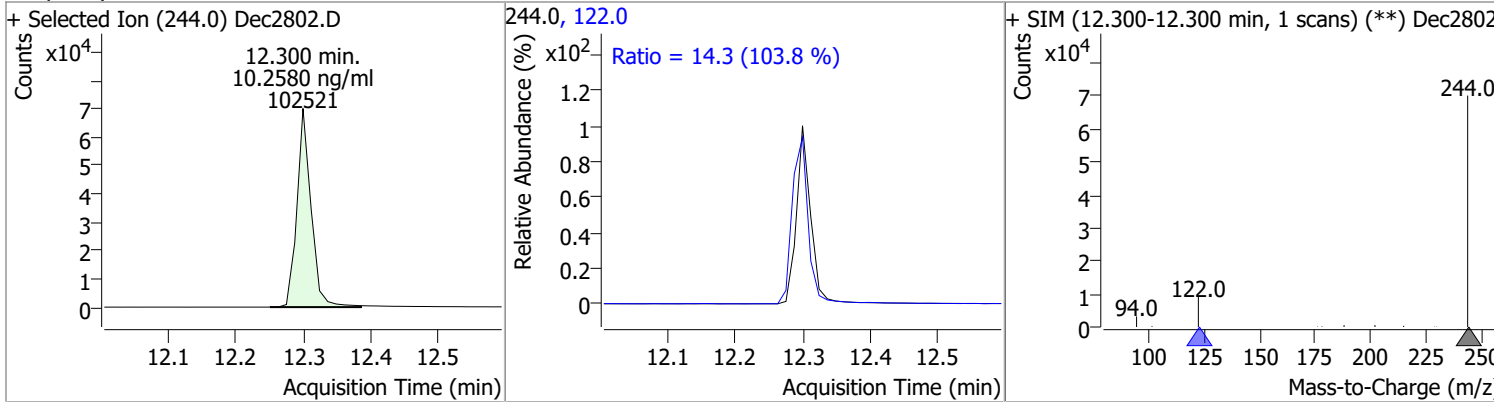

Quantitation Results Report (QT Reviewed)

Data File	Dec2803.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	12/28/2021 6:03:21 PM
Sample Name	28-Dec-21_CAL_6	Instrument	GCMS
Vial	3	Multiplier	1.00
DA Method File		Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	122821 bna SIM 1.batch.bin	Last Calib Update	12/29/2021 8:56:55 AM

Ref Library



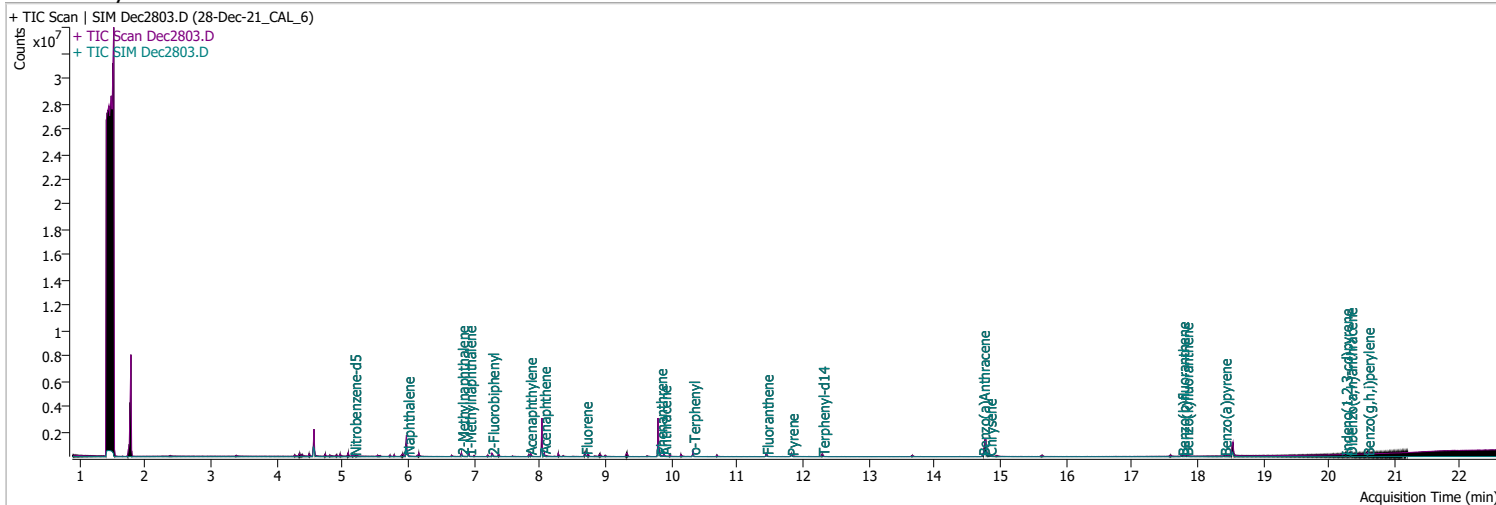


Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
System Monitoring Compounds						
S Nitrobenzene-d5	5.180	82.0	42512	5.1120	ng/ml	m
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 102.24%		*
S 2-Fluorobiphenyl	7.277	172.0	77505	4.6080	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 92.16%		
S Terphenyl-d14	12.300	244.0	48329	4.6204	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 92.41%		
Target Compounds						
T Naphthalene	5.991	128.0	98629	4.8018	ng/ml	98
T 2-Methylnaphthalene	6.815	141.0	54126	4.5693	ng/ml	m
T 1-Methylnaphthalene	6.927	141.0	50414	4.6027	ng/ml	m




(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	5.1120	5.18	-0.01	42512 (m)	54.0	31.3	21.6	40.2
					128.0	21.7	21.3	39.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	4.8018	5.99	0.00	98629	102.0	14.3	0.0	46.6
					129.0	11.2	7.6	14.1




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	4.5693	6.81	0.00	54126 (m)	142.0	148.3	103.3	191.8
					115.0	54.3	36.8	68.3




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	4.6027	6.93	0.00	50414 (m)	142.0	110.5	77.9	144.7
					115.0	63.7	44.4	82.5

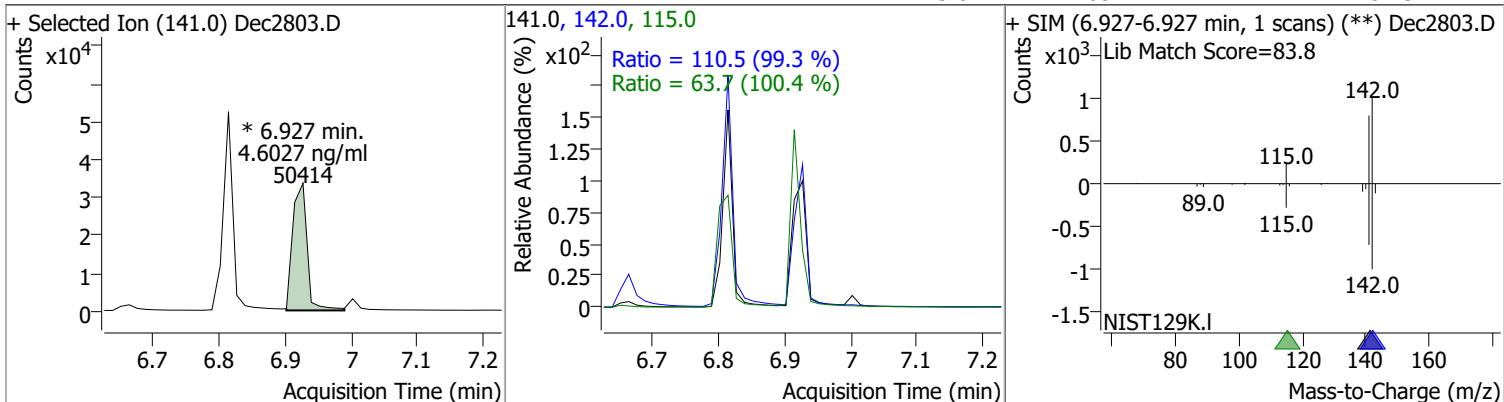

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	4.6080	7.28	0.00	77505	171.0	37.5	26.4	49.0

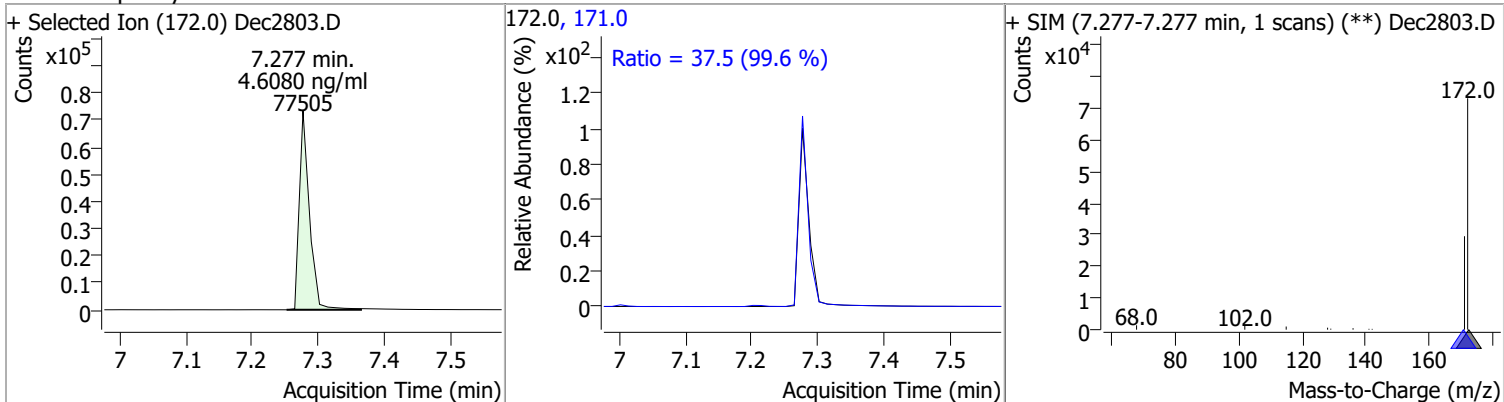


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	4.6204	12.30	0.00	48329	122.0	14.0	9.6	17.9

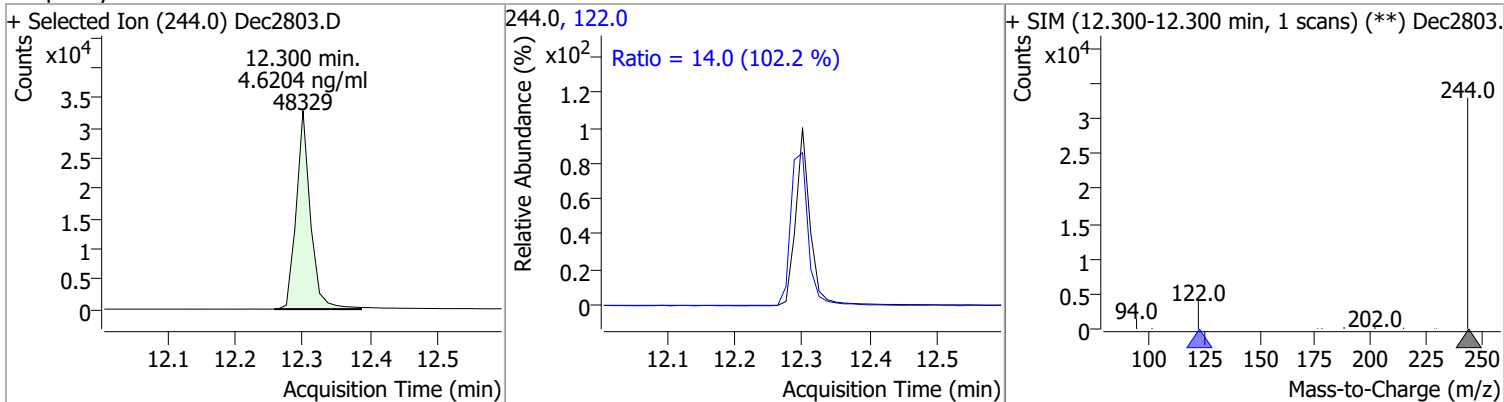

Quantitation Results Report (QT Reviewed)

Data File	Dec2804.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	12/28/2021 6:35:53 PM
Sample Name	28-Dec-21_CAL_5	Instrument	GCMS
Vial	4	Multiplier	1.00
DA Method File		Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	122821 bna SIM 1.batch.bin	Last Calib Update	12/29/2021 8:56:55 AM

Ref Library






Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
System Monitoring Compounds						
S Nitrobenzene-d5	5.193	82.0	14443	1.9208	ng/ml	m
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 38.42%		
S 2-Fluorobiphenyl	7.277	172.0	30043	1.8104	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 36.21%		
S Terphenyl-d14	12.300	244.0	18378	1.8390	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 36.78%		*
Target Compounds						QValue
T Naphthalene	5.991	128.0	37909	1.9031	ng/ml	100
T 2-Methylnaphthalene	6.815	141.0	21520	1.8732	ng/ml	m
T 1-Methylnaphthalene	6.927	141.0	19512	1.8368	ng/ml	m




(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	1.9208	5.19	0.00	14443 (m)	54.0	30.3	21.6	40.2
					128.0	29.8	21.3	39.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	1.9031	5.99	0.00	37909	102.0	15.5	0.0	46.6
					129.0	10.8	7.6	14.1

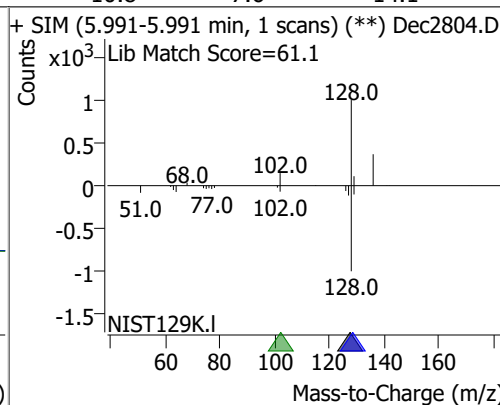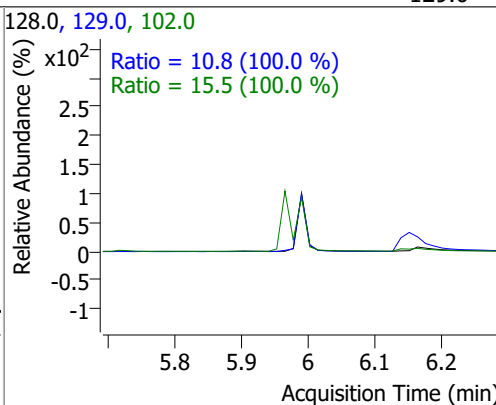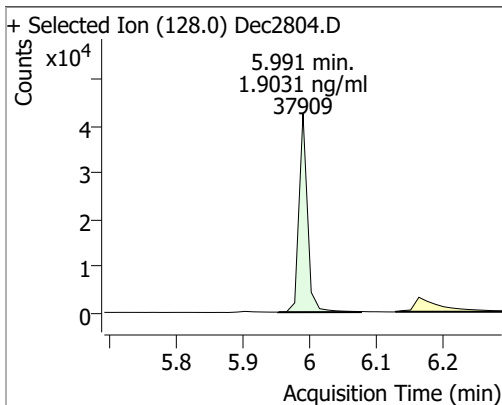


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	1.8732	6.81	0.00	21520 (m)	142.0	147.5	103.3	191.8
					115.0	52.5	36.8	68.3

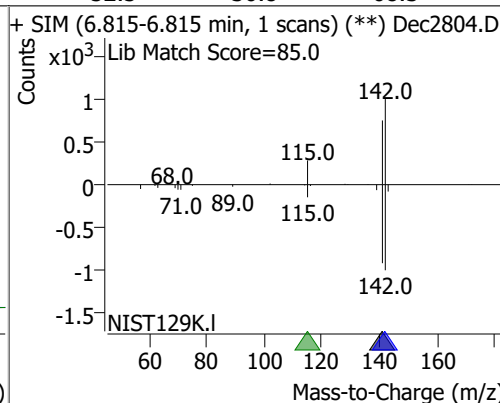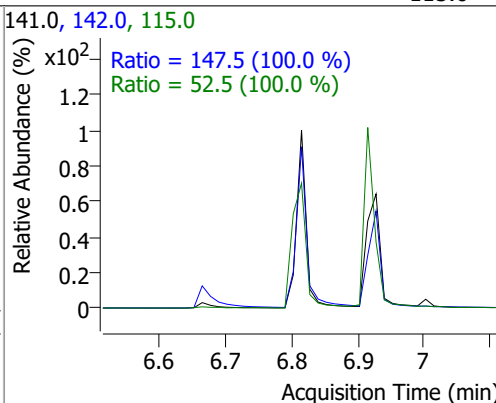


Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	1.8368	6.93	0.00	19512 (m)	142.0	111.3	77.9	144.7
					115.0	63.4	44.4	82.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	1.8104	7.28	0.00	30043	171.0	37.7	26.4	49.0




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	1.8390	12.30	0.00	18378	122.0	13.7	9.6	17.9



Quantitation Results Report (QT Reviewed)

Data File	Dec2805.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	12/28/2021 7:08:33 PM
Sample Name	28-Dec-21_CAL_4	Instrument	GCMS
Vial	5	Multiplier	1.00
DA Method File		Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	122821 bna SIM 1.batch.bin	Last Calib Update	12/29/2021 8:56:55 AM

Ref Library

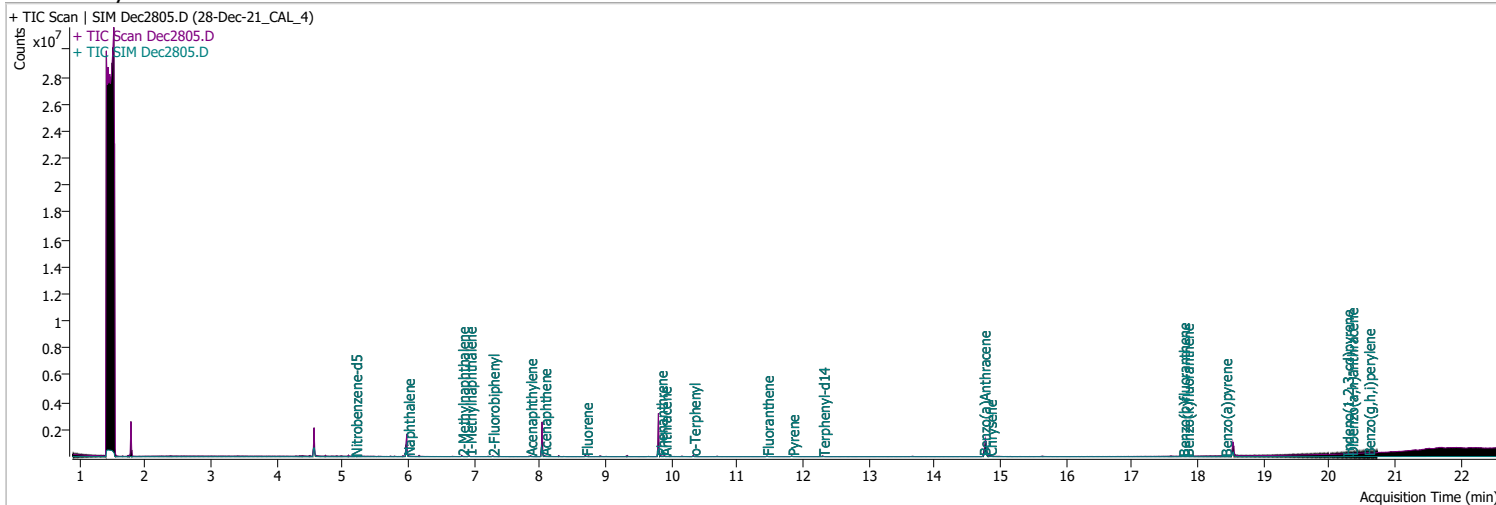


Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
System Monitoring Compounds						
S Nitrobenzene-d5	5.193	82.0	6936	0.9782	ng/ml	0.000
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 19.56%		
S 2-Fluorobiphenyl	7.277	172.0	15555	0.9850	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 19.70%		*
S Terphenyl-d14	12.300	244.0	9183	0.9560	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 19.12%		*
Target Compounds						
T Naphthalene	5.991	128.0	19154	0.9908	ng/ml	98
T 2-Methylnaphthalene	6.815	141.0	10932	0.9806	ng/ml	95
T 1-Methylnaphthalene	6.927	141.0	9969	0.9670	ng/ml	99


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	0.9782	5.19	0.00	6936	54.0	31.2	21.6	40.2
					128.0	31.1	21.3	39.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	0.9908	5.99	0.00	19154	102.0	16.9	0.0	46.6
					129.0	11.0	7.6	14.1




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	0.9806	6.81	0.00	10932	142.0	142.6	103.3	191.8
					115.0	45.7	36.8	68.3




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	0.9670	6.93	0.00	9969	142.0	109.9	77.9	144.7
					115.0	62.8	44.4	82.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	0.9850	7.28	0.00	15555	171.0	36.6	26.4	49.0




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	0.9560	12.30	0.00	9183	122.0	14.6	9.6	17.9



Quantitation Results Report (QT Reviewed)

Data File	Dec2806.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	12/28/2021 7:41:06 PM
Sample Name	28-Dec-21_CAL_3	Instrument	GCMS
Vial	6	Multiplier	1.00
DA Method File		Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	122821 bna SIM 1.batch.bin	Last Calib Update	12/29/2021 8:56:55 AM

Ref Library






Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
System Monitoring Compounds						
S Nitrobenzene-d5	5.193	82.0	3113	0.5197	ng/ml	0.000
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 10.39%		*
S 2-Fluorobiphenyl	7.277	172.0	7476	0.4977	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 9.95%		*
S Terphenyl-d14	12.300	244.0	4385	0.4985	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 9.97%		*
Target Compounds						
T Naphthalene	5.991	128.0	9084	0.4974	ng/ml	96
T 2-Methylnaphthalene	6.815	141.0	5515	0.5236	ng/ml	94
T 1-Methylnaphthalene	6.927	141.0	4850	0.4980	ng/ml	98




(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	0.5197	5.19	0.00	3113	54.0	30.2	21.6	40.2
					128.0	32.6	21.3	39.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	0.4974	5.99	0.00	9084	102.0	18.0	0.0	46.6
					129.0	10.5	7.6	14.1




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	0.5236	6.81	0.00	5515	142.0	139.3	103.3	191.8
					115.0	48.4	36.8	68.3




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	0.4980	6.93	0.00	4850	142.0	109.3	77.9	144.7
					115.0	65.8	44.4	82.5

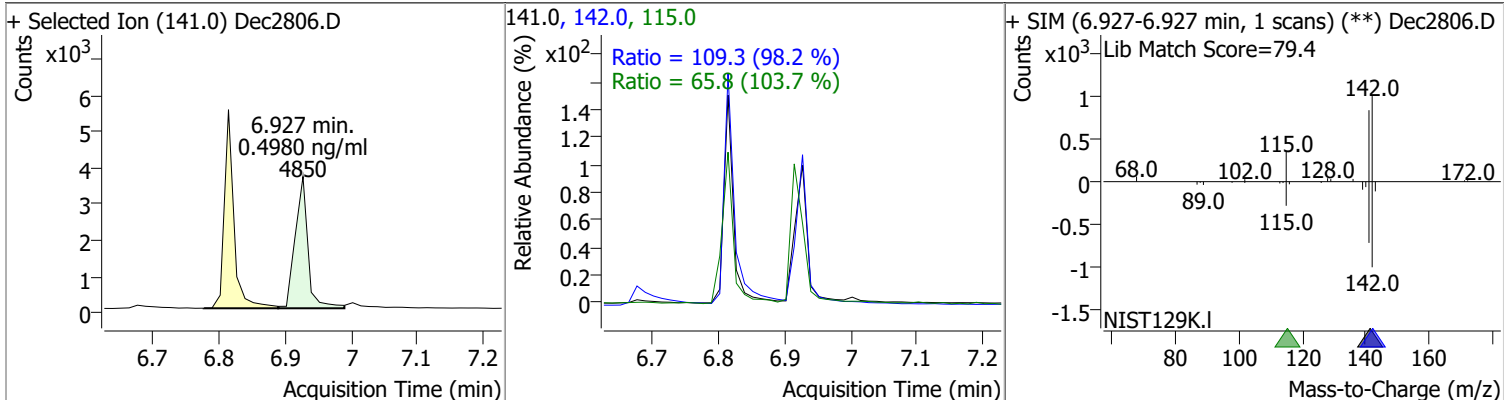

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	0.4977	7.28	0.00	7476	171.0	35.2	26.4	49.0

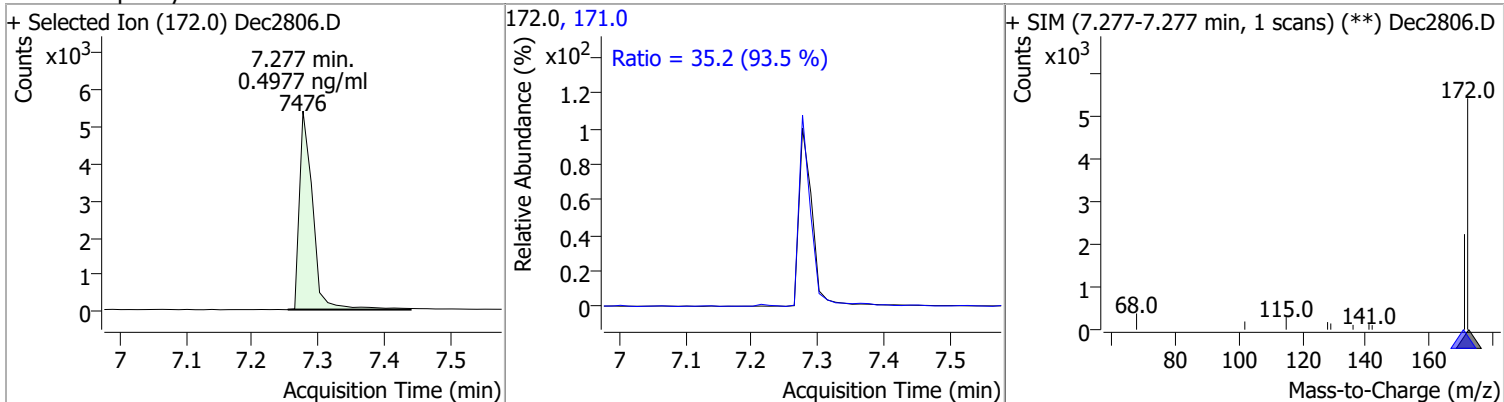


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	0.4985	12.30	0.00	4385	122.0	14.8	9.6	17.9



Quantitation Results Report (QT Reviewed)

Data File	Dec2807.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	12/28/2021 8:13:46 PM
Sample Name	28-Dec-21_CAL_2	Instrument	GCMS
Vial	7	Multiplier	1.00
DA Method File		Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	122821 bna SIM 1.batch.bin	Last Calib Update	12/29/2021 8:56:55 AM

Ref Library




Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
System Monitoring Compounds						
S Nitrobenzene-d5	5.205	82.0	1083	0.1999	ng/ml	0.012
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 4.00%		*
S 2-Fluorobiphenyl	7.277	172.0	3084	0.2125	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 4.25%		*
S Terphenyl-d14	12.300	244.0	1955	0.2059	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 4.12%		*
Target Compounds						
T Naphthalene	5.991	128.0	3569	0.1946	ng/ml	88
T 2-Methylnaphthalene	6.815	141.0	2170	0.2052	ng/ml	96
T 1-Methylnaphthalene	6.927	141.0	2021	0.2066	ng/ml	94


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	0.1999	5.21	0.01	1083	54.0	29.7	21.6	40.2
					128.0	29.7	21.3	39.5

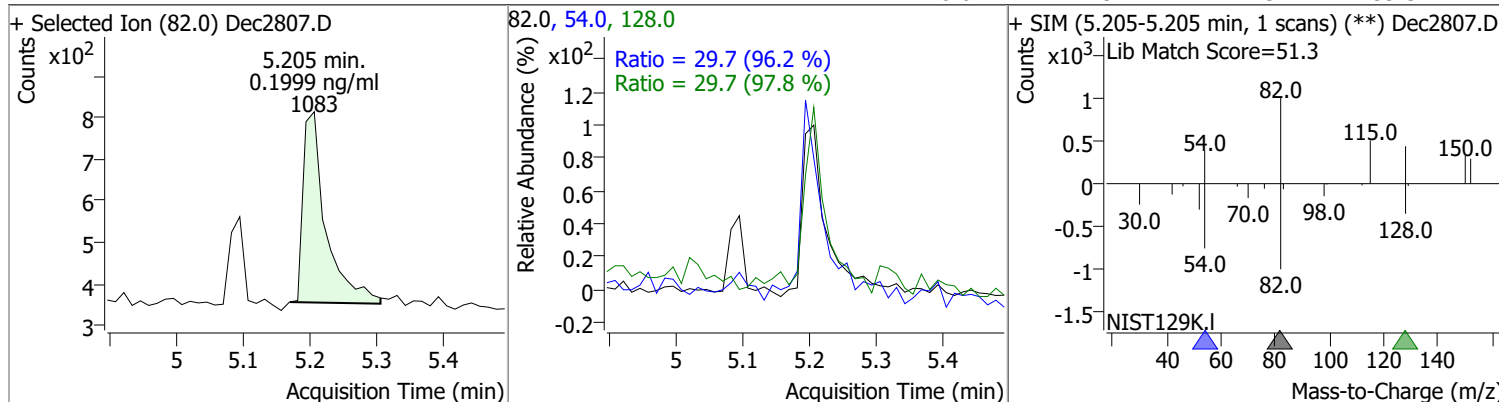

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	0.1946	5.99	0.00	3569	102.0	23.5	0.0	46.6
					129.0	11.1	7.6	14.1

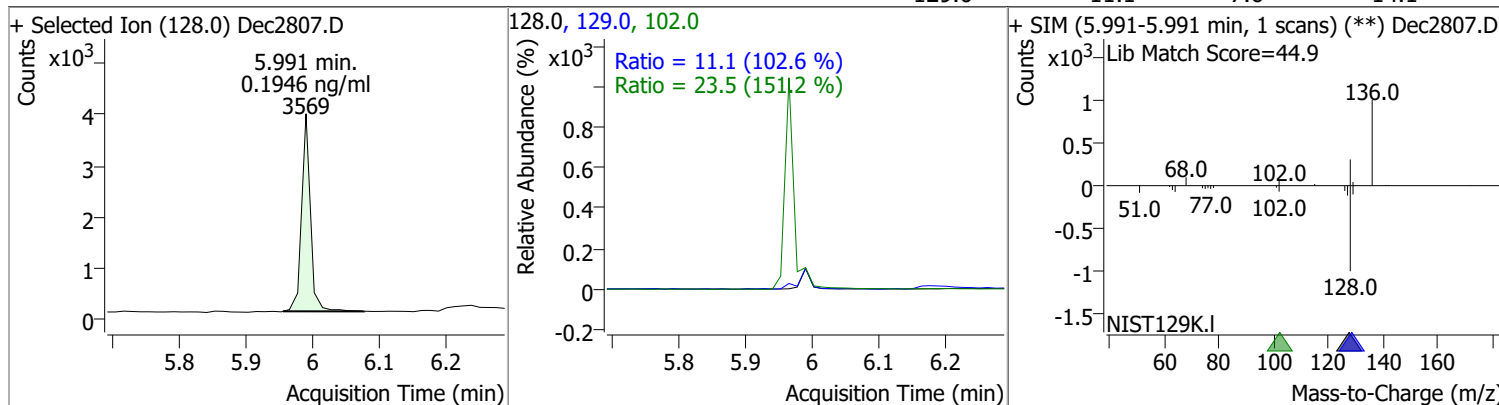


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	0.2052	6.81	0.00	2170	142.0	141.7	103.3	191.8
					115.0	51.7	36.8	68.3

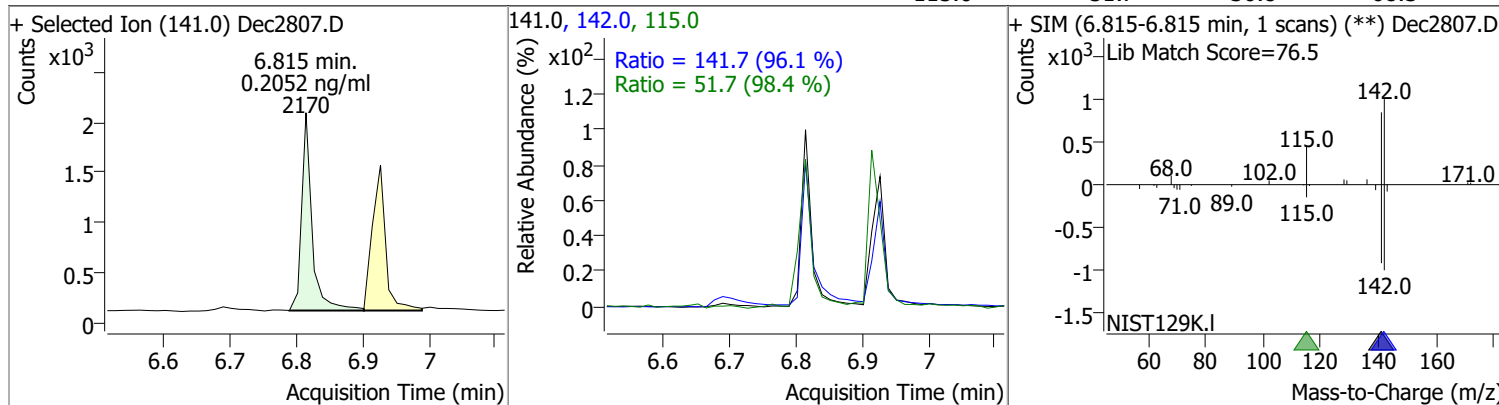


Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	0.2066	6.93	0.00	2021	142.0	106.1	77.9	144.7
					115.0	56.3	44.4	82.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	0.2125	7.28	0.00	3084	171.0	36.4	26.4	49.0




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	0.2059	12.30	0.00	1955	122.0	13.4	9.6	17.9



Quantitation Results Report (QT Reviewed)

Data File	Dec2808.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	12/28/2021 8:46:23 PM
Sample Name	28-Dec-21_CAL_1	Instrument	GCMS
Vial	8	Multiplier	1.00
DA Method File		Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	122821 bna SIM 1.batch.bin	Last Calib Update	12/29/2021 8:56:55 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
----------	----	------	-------	-------	-------	----------

Internal Standards

System Monitoring Compounds

S Nitrobenzene-d5	5.205	82.0	515	0.1003	ng/ml	0.012
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 2.01%		*
S 2-Fluorobiphenyl	7.277	172.0	1855	0.1181	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 2.36%		*
S Terphenyl-d14	12.300	244.0	1041	0.1148	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 2.30%		*


Target Compounds

Compound	RT	QIon	Resp.	Conc.	Units	QValue
T Naphthalene	5.991	128.0	2075	0.1077	ng/ml	82
T 2-Methylnaphthalene	6.815	141.0	1176	0.1059	ng/ml	97
T 1-Methylnaphthalene	6.927	141.0	1191	0.1159	ng/ml	99


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	0.1003	5.21	0.01	515	54.0 128.0	30.6 22.5	21.6 21.3	40.2 39.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	0.1077	5.99	0.00	2075	102.0 129.0	28.2 11.0	0.0 7.6	46.6 14.1




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	0.1059	6.81	0.00	1176	142.0 115.0	150.0 48.0	103.3 36.8	191.8 68.3

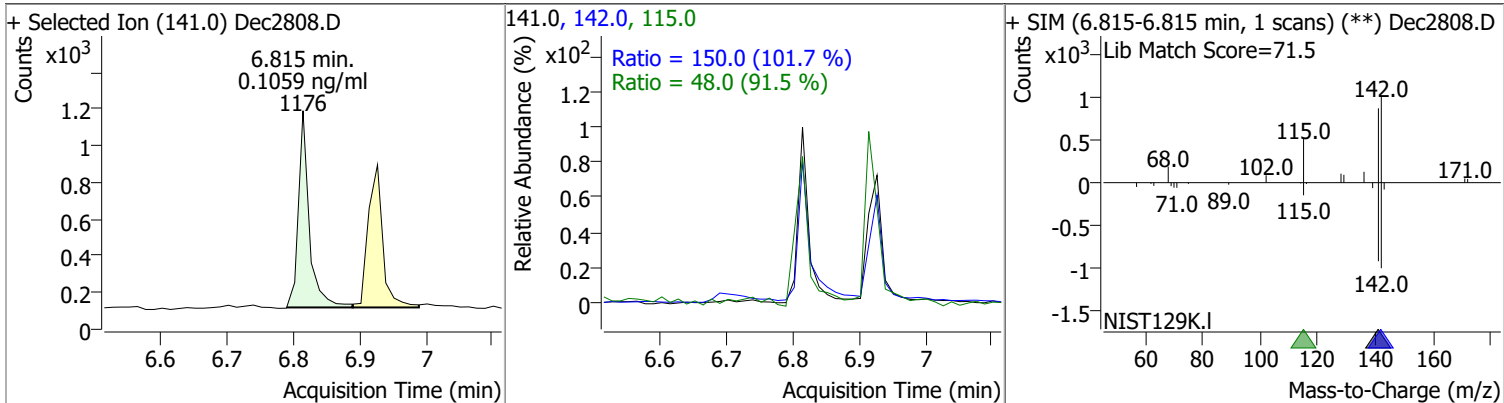


Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	0.1159	6.93	0.00	1191	142.0	109.9	77.9	144.7
					115.0	62.0	44.4	82.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	0.1181	7.28	0.00	1855	171.0	35.9	26.4	49.0




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	0.1148	12.30	0.00	1041	122.0	15.4	9.6	17.9



Quantitation Results Report (QT Reviewed)

Data File	Dec2809.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	12/28/2021 9:19:01 PM
Sample Name	28-Dec-21_CCV_9	Instrument	GCMS
Vial	9	Multiplier	1.00
DA Method File		Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	122821 bna SIM 1.batch.bin	Last Calib Update	12/29/2021 8:56:55 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
----------	----	------	-------	-------	-------	----------

Internal Standards

System Monitoring Compounds

S Nitrobenzene-d5	5.181	82.0	18569	2.3877	ng/ml	-0.012
Spiked Amount: 5.000	Range: 19.0 - 102.0%		Recovery = 47.75%			
S 2-Fluorobiphenyl	7.277	172.0	38269	2.2626	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%		Recovery = 45.25%			
S Terphenyl-d14	12.288	244.0	21623	1.9390	ng/ml	-0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%		Recovery = 38.78%		*	




Target Compounds

Compound	RT	QIon	Resp.	Conc.	Units	QValue
T Naphthalene	5.991	128.0	44031	2.0586	ng/ml	96
T 2-Methylnaphthalene	6.815	141.0	26021	2.1095	ng/ml	97
T 1-Methylnaphthalene	6.915	141.0	26026	2.2818	ng/ml	98




(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	2.3877	5.18	-0.01	18569	54.0	31.6	21.6	40.2
					128.0	25.7	21.3	39.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	2.0586	5.99	0.00	44031	102.0	13.3	0.0	46.6
					129.0	11.5	7.6	14.1




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	2.1095	6.81	0.00	26021	142.0	146.6	103.3	191.8
					115.0	59.0	36.8	68.3




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	2.2818	6.91	-0.01	26026	142.0	113.6	77.9	144.7
					115.0	62.9	44.4	82.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	2.2626	7.28	0.00	38269	171.0	36.8	26.4	49.0




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	1.9390	12.29	-0.01	21623	122.0	14.5	9.6	17.9



Quantitation Results Report (QT Reviewed)

Data File	Dec2810.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	12/28/2021 9:51:35 PM
Sample Name	28-Dec-21_ISTBLK_10	Instrument	GCMS
Vial	10	Multiplier	1.00
DA Method File		Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	122821 bna SIM 1.batch.bin	Last Calib Update	12/29/2021 8:56:55 AM

Ref Library

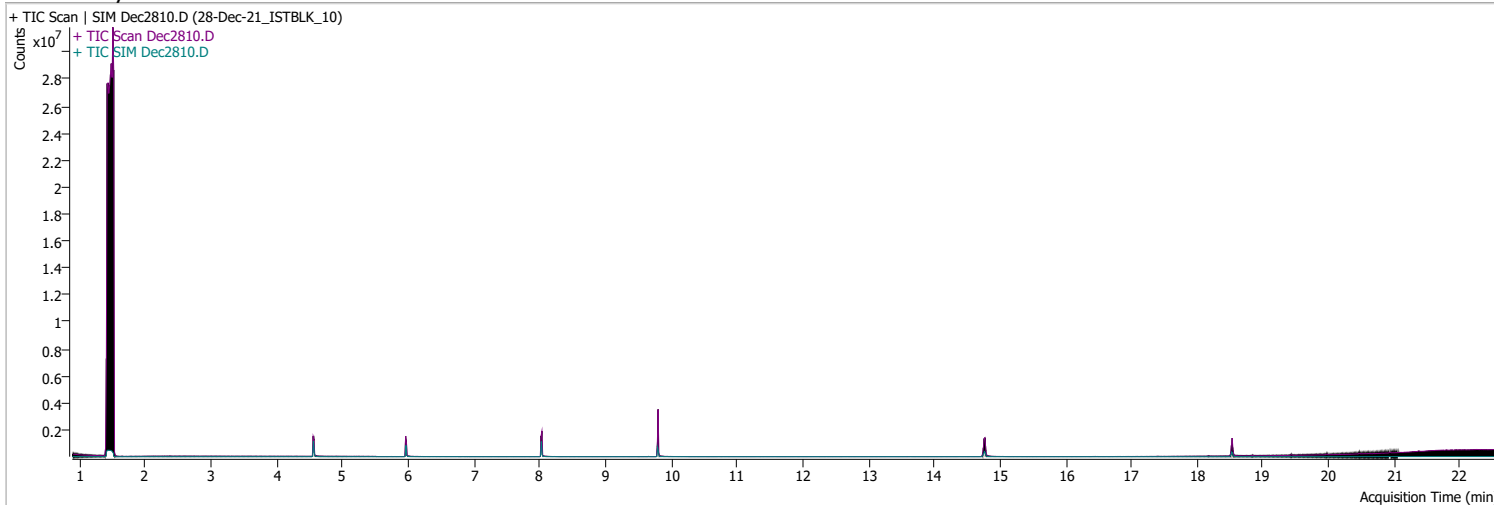

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
----------	----	------	-------	-------	-------	----------

Internal Standards

System Monitoring Compounds





S Nitrobenzene-d5	0.000	0	N.D.
Spiked Amount: 5.000	Range: 19.0 - 102.0%		Recovery = NA%
S 2-Fluorobiphenyl	0.000	0	N.D.
Spiked Amount: 5.000	Range: 25.0 - 94.0%		Recovery = NA%
S Terphenyl-d14	0.000	0	N.D.
Spiked Amount: 5.000	Range: 39.0 - 106.0%		Recovery = NA%

Target Compounds

Target Compounds	RT	QIon	Resp.	Conc.	Units	QValue
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)

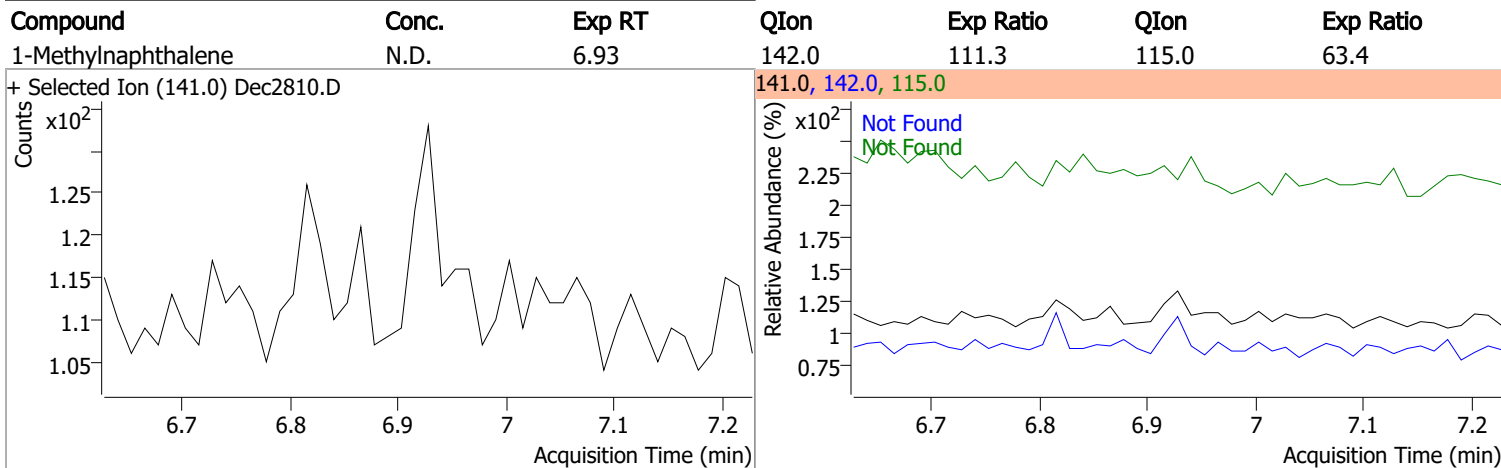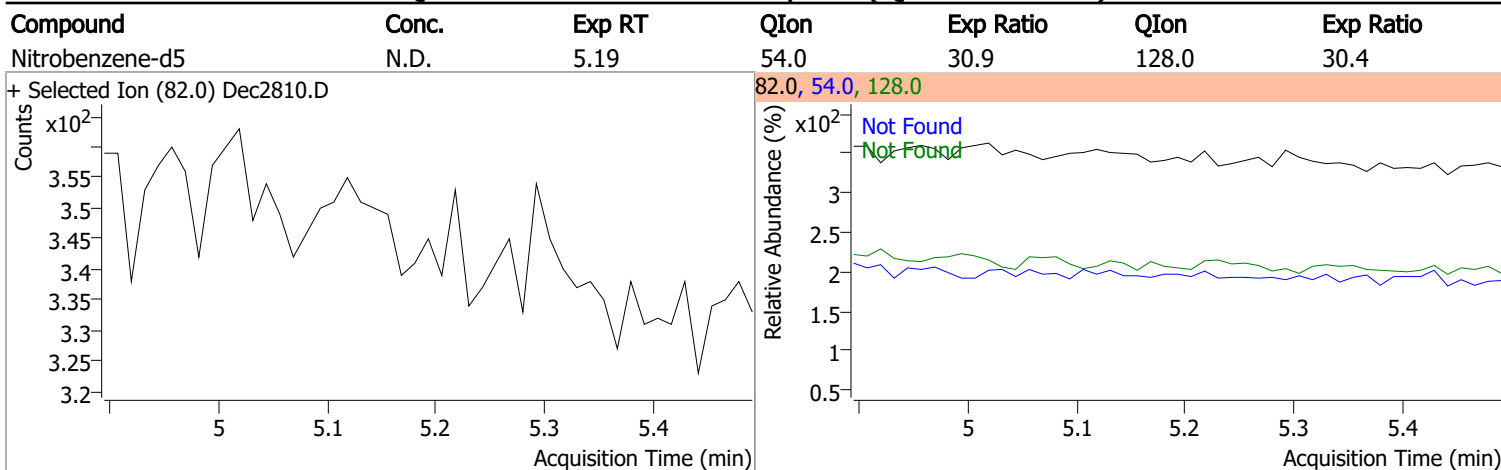


Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio
2-Fluorobiphenyl	N.D.	7.28	171.0	37.7

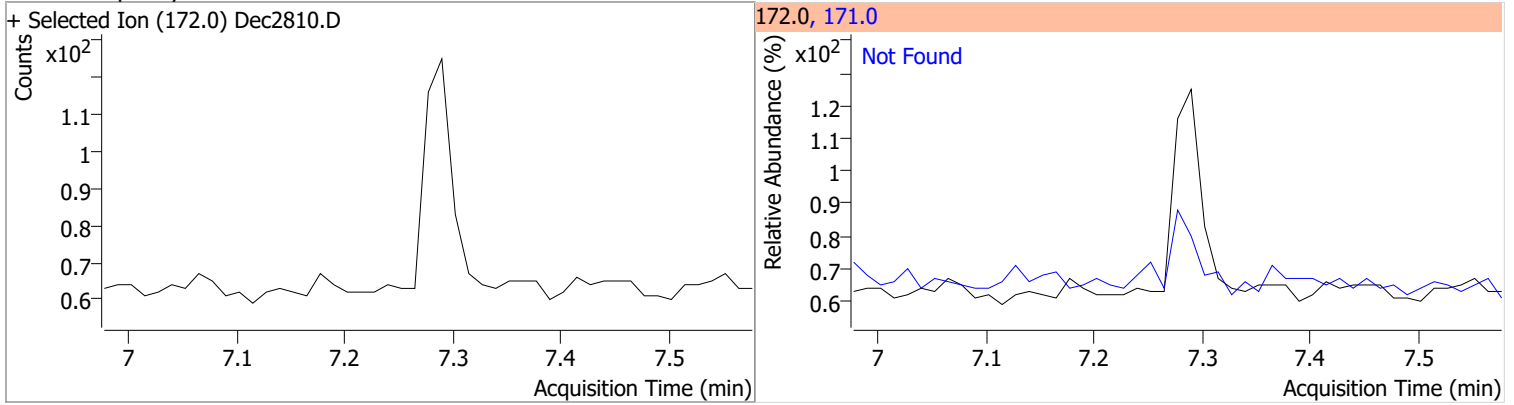


Compound	Conc.	Exp RT	QIon	Exp Ratio
Terphenyl-d14	N.D.	12.30	122.0	13.7

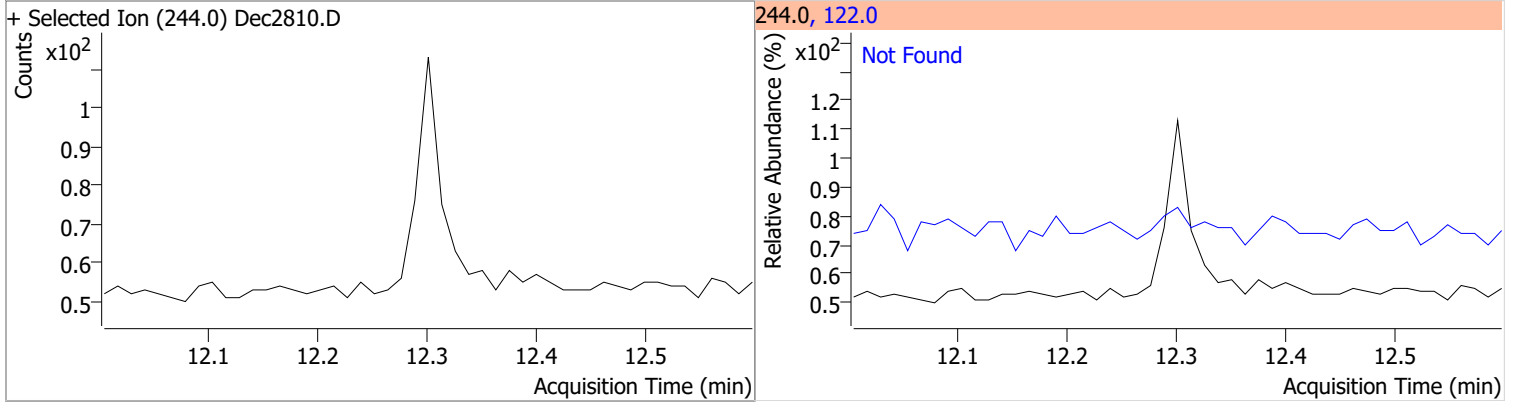

Quantitation Results Report (QT Reviewed)

Data File	Dec2811.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	12/28/2021 10:24:13 PM
Sample Name	MB-162432	Instrument	GCMS
Vial	11	Multiplier	1.00
DA Method File		Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	122821 bna SIM 1.batch.bin	Last Calib Update	12/29/2021 8:56:55 AM

Ref Library

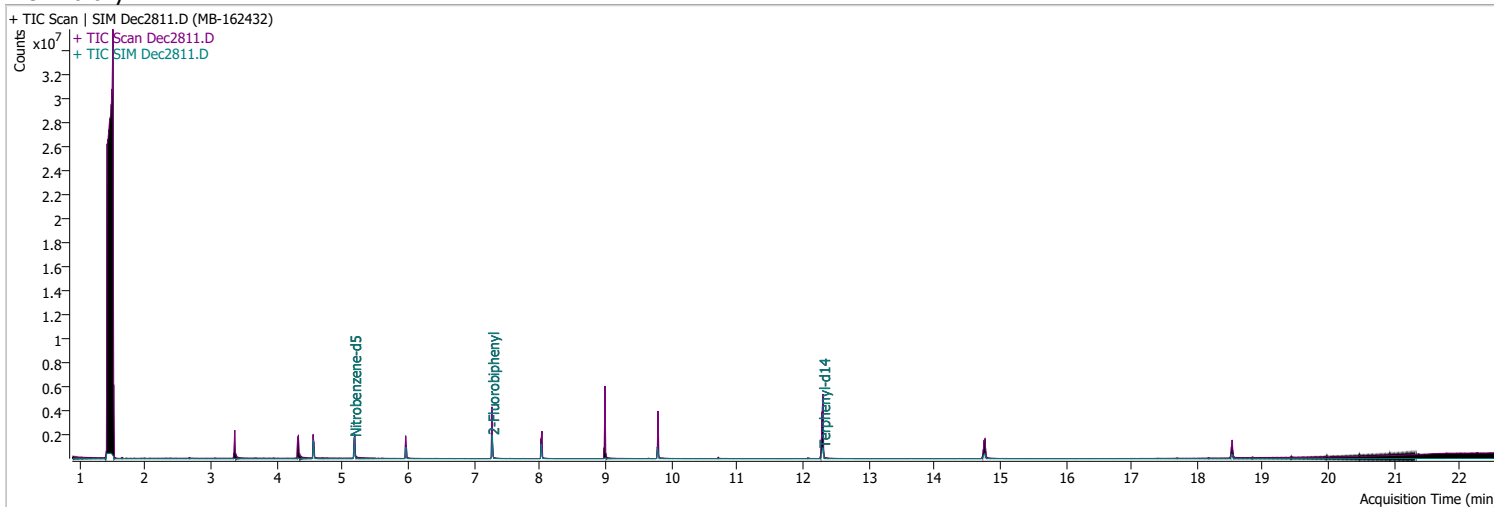


Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
System Monitoring Compounds						
S Nitrobenzene-d5	5.181	82.0	1003127	48.1837	ng/ml	-0.012
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 963.67%		*
S 2-Fluorobiphenyl	7.277	172.0	1232820	60.8518	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1217.04%		*
S Terphenyl-d14	12.313	244.0	1460555	114.7615	ng/ml	0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 2295.23%		*
Target Compounds						QValue
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	48.1837	5.18	-0.01	1003127	54.0	33.4	21.6	40.2
					128.0	27.2	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.99	102.0	15.5	129.0	10.8



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.81	142.0	147.5	115.0	52.5






Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.93	142.0	111.3	115.0	63.4






Quantitation Results Report (QT Reviewed)

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	60.8518	7.28	0.00	1232820	171.0	40.6	26.4	49.0

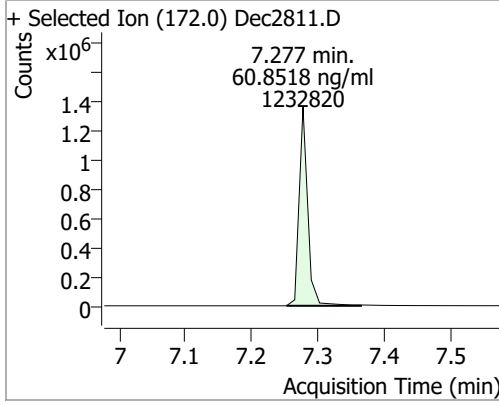


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	114.7615	12.31	0.01	1460555	122.0	14.4	9.6	17.9



Quantitation Results Report (QT Reviewed)

Data File	Dec2812.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	12/28/2021 10:56:47 PM
Sample Name	MB-162432	Instrument	GCMS
Vial	12	Multiplier	20.00
DA Method File		Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	122821 bna SIM 1.batch.bin	Last Calib Update	12/29/2021 8:56:55 AM

Ref Library

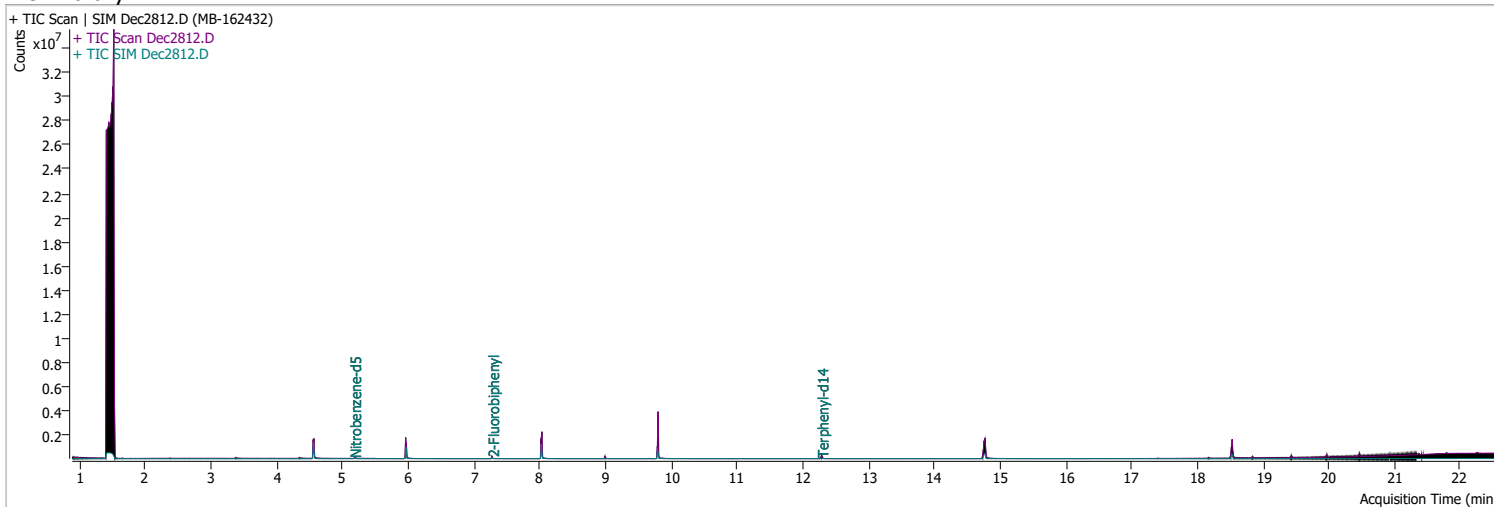

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
----------	----	------	-------	-------	-------	----------

Internal Standards

System Monitoring Compounds

S Nitrobenzene-d5	5.181	82.0	35606	74.3801	ng/ml	-0.012
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 1487.60%		*
S 2-Fluorobiphenyl	7.277	172.0	68112	67.0874	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1341.75%		*
S Terphenyl-d14	12.288	244.0	64004	97.9428	ng/ml	-0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 1958.86%		*


Target Compounds

Target Compounds	RT	QIon	Resp.	Conc.	Units	QValue
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	74.3801	5.18	-0.01	35606	54.0	22.3	21.6	40.2
					128.0	25.5	21.3	39.5

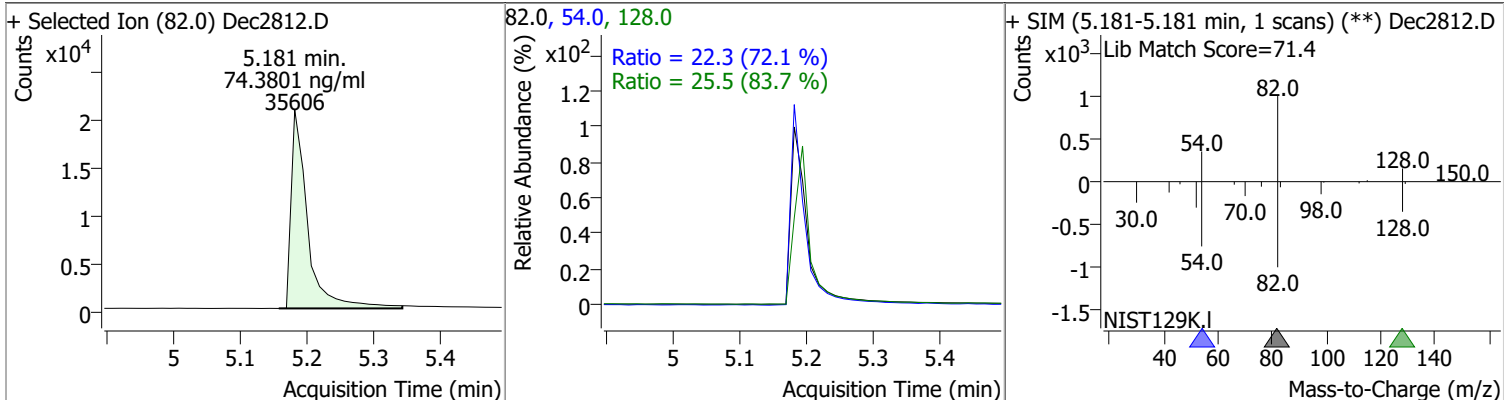


Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.99	102.0	15.5	129.0	10.8

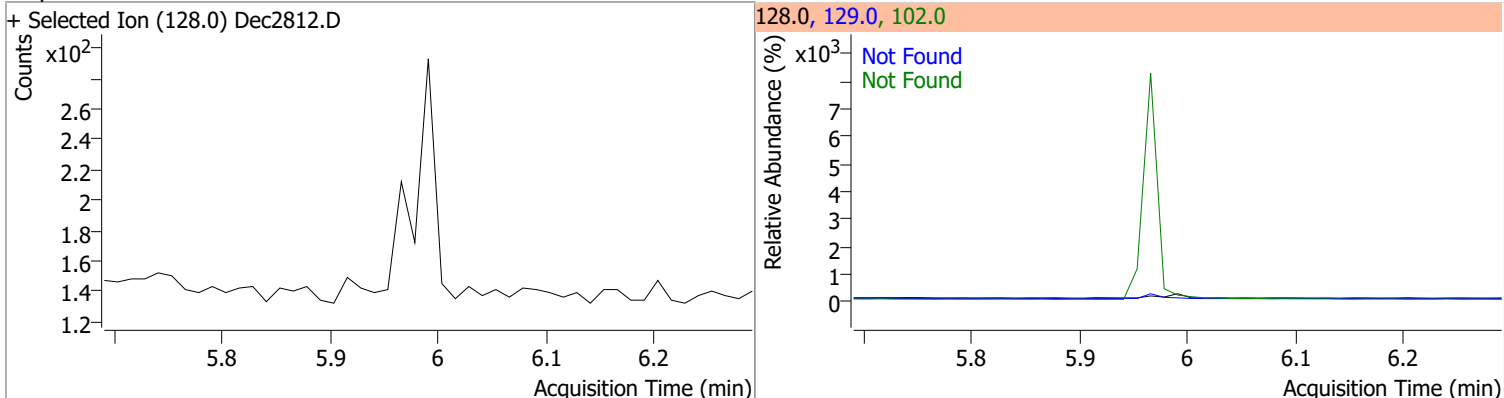

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.81	142.0	147.5	115.0	52.5



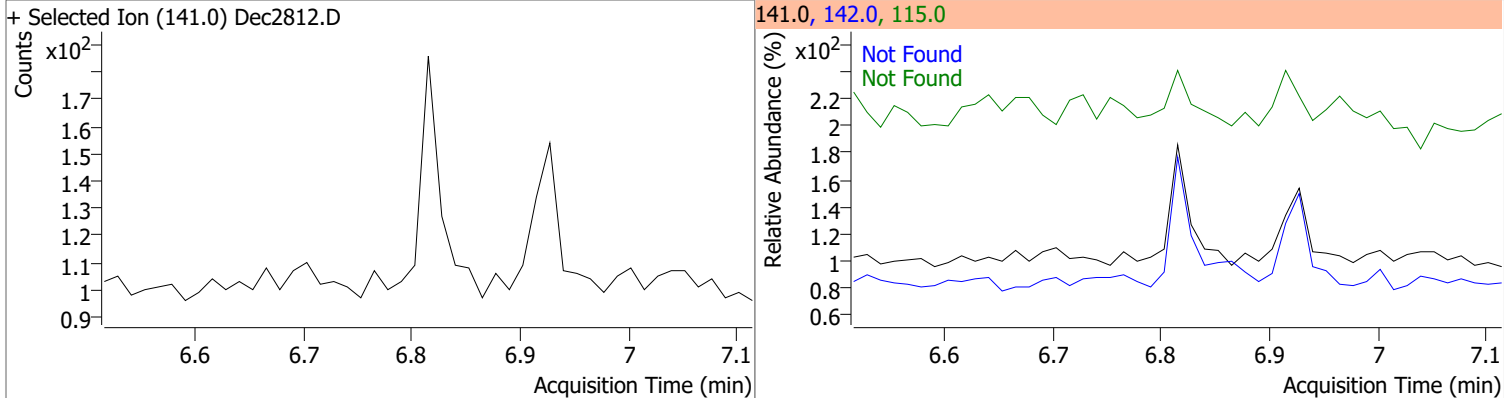


Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.93	142.0	111.3	115.0	63.4



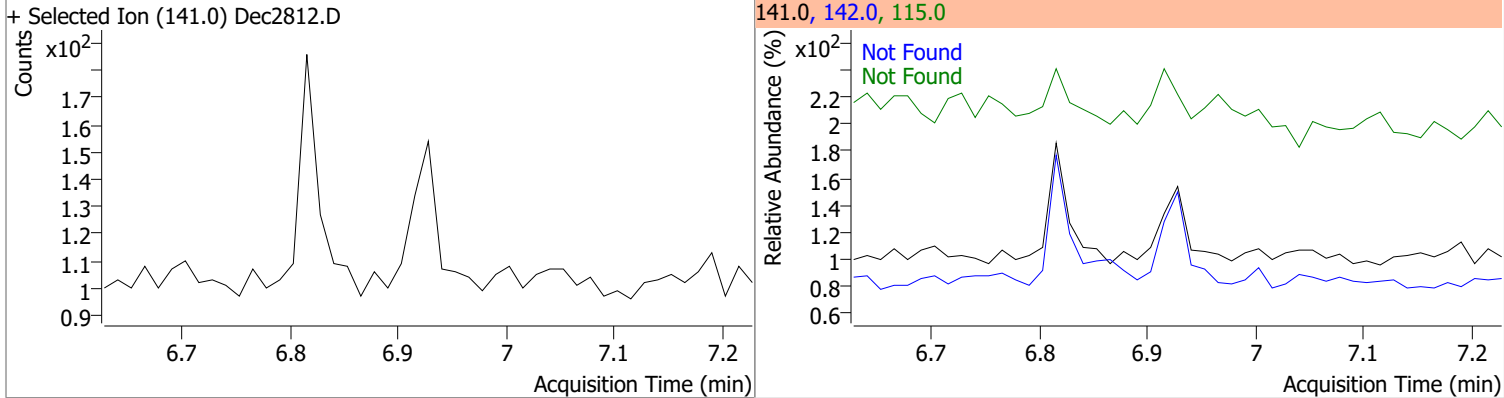


Quantitation Results Report (QT Reviewed)

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	67.0874	7.28	0.00	68112	171.0	35.9	26.4	49.0

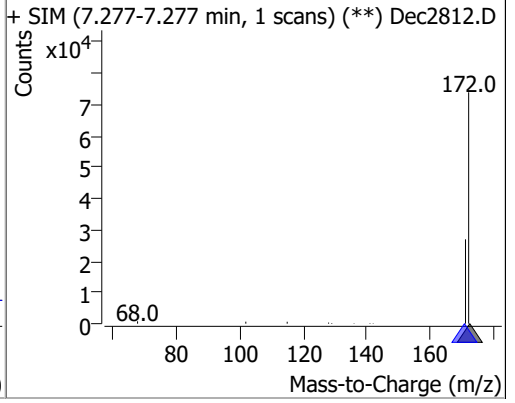


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	97.9428	12.29	-0.01	64004	122.0	14.5	9.6	17.9

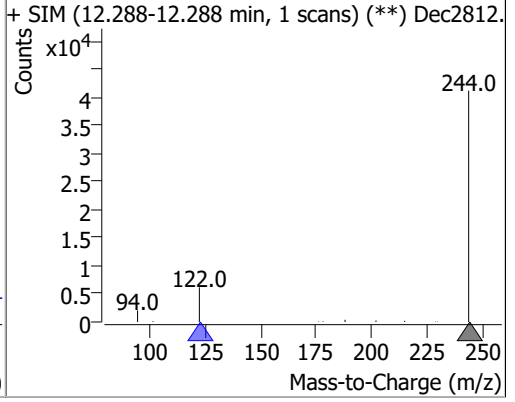

Quantitation Results Report (QT Reviewed)

Data File	Dec2813.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	12/28/2021 11:29:26 PM
Sample Name	LLCS-162432	Instrument	GCMS
Vial	13	Multiplier	1.00
DA Method File		Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	122821 bna SIM 1.batch.bin	Last Calib Update	12/29/2021 8:56:55 AM

Ref Library



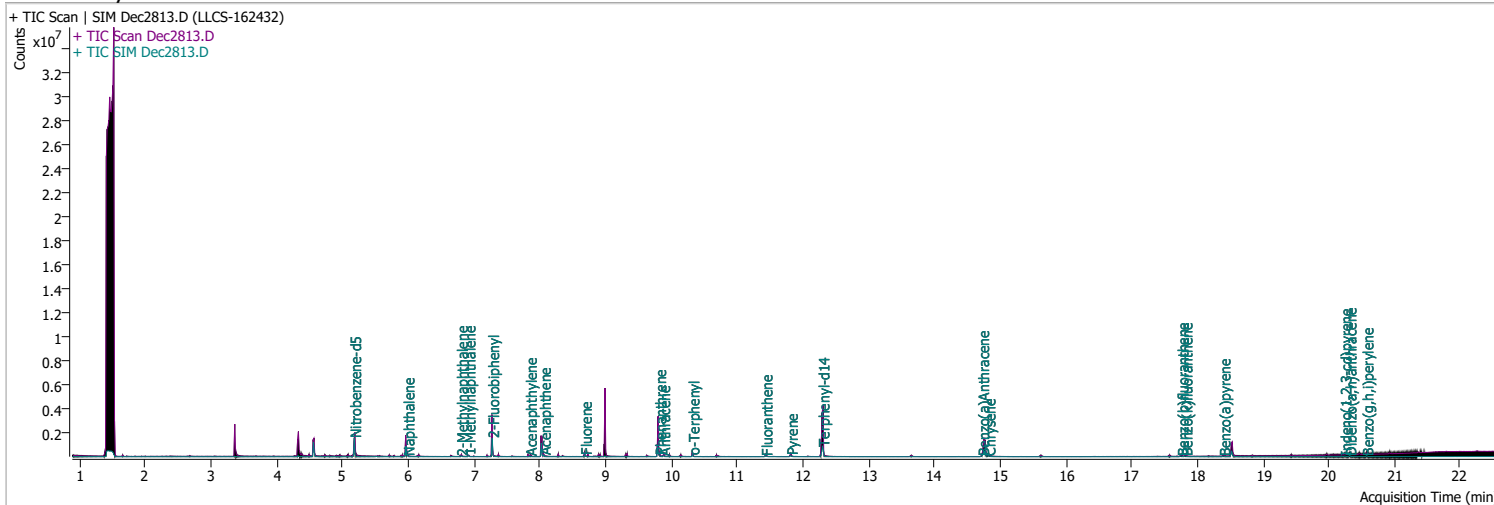


Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
System Monitoring Compounds						
S Nitrobenzene-d5	5.181	82.0	895211	49.7814	ng/ml	-0.012
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 995.63%		*
S 2-Fluorobiphenyl	7.277	172.0	934338	51.3804	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1027.61%		*
S Terphenyl-d14	12.300	244.0	1248436	106.1419	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 2122.84%		*
Target Compounds						
T Naphthalene	5.991	128.0	59261	2.5629	ng/ml	95
T 2-Methylnaphthalene	6.802	141.0	35999	2.6995	ng/ml	89
T 1-Methylnaphthalene	6.915	141.0	37319	3.0265	ng/ml	98




(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	49.7814	5.18	-0.01	895211	54.0	33.5	21.6	40.2
					128.0	25.7	21.3	39.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	2.5629	5.99	0.00	59261	102.0	12.4	0.0	46.6
					129.0	11.3	7.6	14.1






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	2.6995	6.80	-0.01	35999	142.0	160.3	103.3	191.8
					115.0	62.6	36.8	68.3






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	3.0265	6.91	-0.01	37319	142.0	110.5	77.9	144.7
					115.0	60.5	44.4	82.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	51.3804	7.28	0.00	934338	171.0	39.8	26.4	49.0




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	106.1419	12.30	0.00	1248436	122.0	14.8	9.6	17.9



Quantitation Results Report (QT Reviewed)

Data File	Dec2814.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	12/29/2021 12:01:58 AM
Sample Name	LLCS-162432	Instrument	GCMS
Vial	14	Multiplier	20.00
DA Method File		Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	122821 bna SIM 1.batch.bin	Last Calib Update	12/29/2021 8:56:55 AM

Ref Library






Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
System Monitoring Compounds						
S Nitrobenzene-d5	5.180	82.0	23331	62.7180	ng/ml	-0.013
Spiked Amount: 5.000				Recovery = 1254.36%		*
S 2-Fluorobiphenyl	7.277	172.0	46619	54.2288	ng/ml	0.000
Spiked Amount: 5.000				Recovery = 1084.58%		*
S Terphenyl-d14	12.288	244.0	54531	111.7317	ng/ml	-0.012
Spiked Amount: 5.000				Recovery = 2234.63%		*
Target Compounds						QValue
T Naphthalene	5.991	128.0	2879	2.7826	ng/ml	87
T 2-Methylnaphthalene	6.815	141.0	1724	2.8888	ng/ml	m 89
T 1-Methylnaphthalene	6.915	141.0	1867	3.3838	ng/ml	m 92




(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	62.7180	5.18	-0.01	23331	54.0	29.5	21.6	40.2
					128.0	31.9	21.3	39.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	2.7826	5.99	0.00	2879	102.0	24.1	0.0	46.6
					129.0	9.6	7.6	14.1




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	2.8888	6.81	0.00	1724 (m)	142.0	133.7	103.3	191.8
					115.0	44.6	36.8	68.3




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	3.3838	6.91	-0.01	1867 (m)	142.0	102.7	77.9	144.7
					115.0	58.1	44.4	82.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	54.2288	7.28	0.00	46619	171.0	35.3	26.4	49.0




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	111.7317	12.29	-0.01	54531	122.0	14.3	9.6	17.9



Quantitation Results Report (QT Reviewed)

Data File	Dec2815.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	12/29/2021 12:34:41 AM
Sample Name	LLCSD-162432	Instrument	GCMS
Vial	15	Multiplier	1.00
DA Method File		Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	122821 bna SIM 1.batch.bin	Last Calib Update	12/29/2021 8:56:55 AM

Ref Library

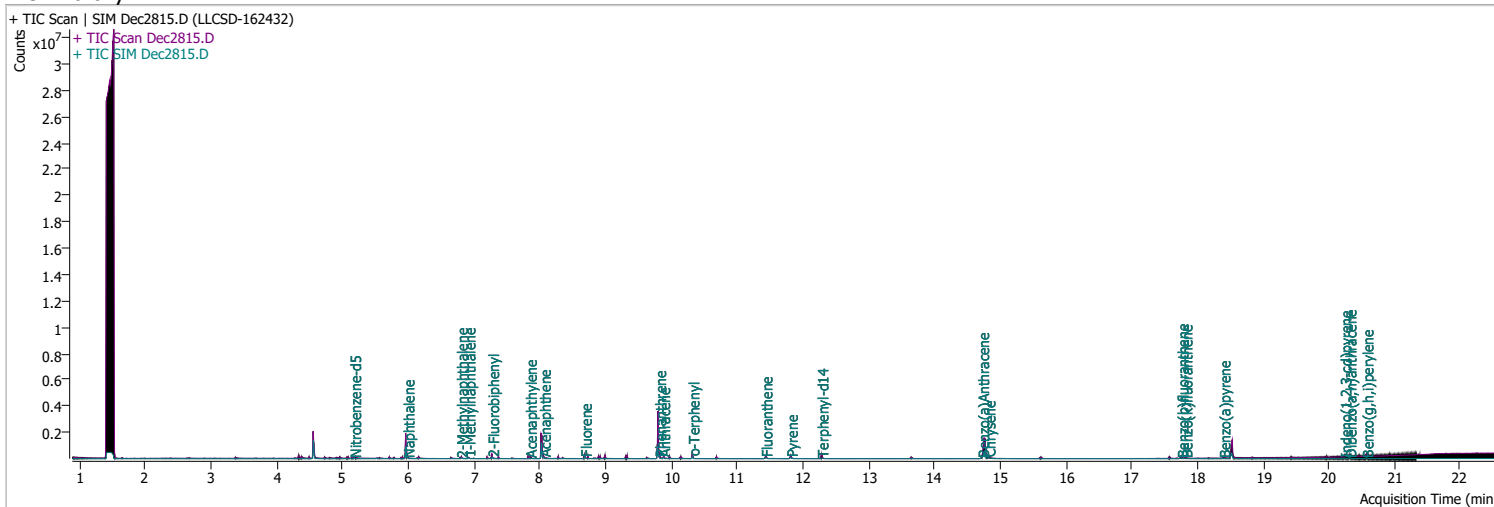

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
----------	----	------	-------	-------	-------	----------

Internal Standards

System Monitoring Compounds

S Nitrobenzene-d5	5.180	82.0	52396	5.3594	ng/ml	-0.013
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 107.19%		*
S 2-Fluorobiphenyl	7.277	172.0	84714	4.2994	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 85.99%		
S Terphenyl-d14	12.288	244.0	81092	6.6526	ng/ml	-0.013
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 133.05%		*




Target Compounds

Compound	RT	QIon	Resp.	Conc.	Units	QValue
T Naphthalene	5.991	128.0	50520	2.0325	ng/ml	95
T 2-Methylnaphthalene	6.802	141.0	31472	2.1956	ng/ml	83
T 1-Methylnaphthalene	6.915	141.0	32536	2.4546	ng/ml	99




(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	5.3594	5.18	-0.01	52396	54.0 128.0	28.9 27.4	21.6 21.3	40.2 39.5

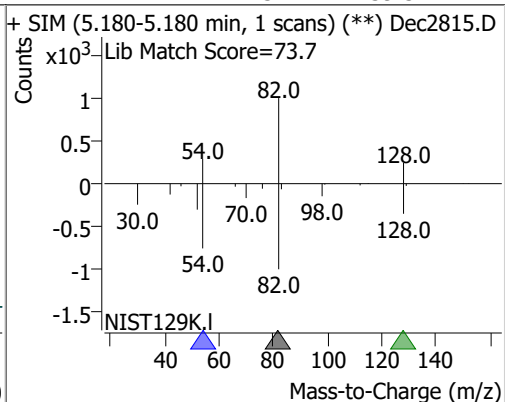

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	2.0325	5.99	0.00	50520	102.0 129.0	12.3 11.4	0.0 7.6	46.6 14.1




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	2.1956	6.80	-0.01	31472	142.0 115.0	170.8 62.4	103.3 36.8	191.8 68.3




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	2.4546	6.91	-0.01	32536	142.0	111.3	77.9	144.7
					115.0	60.4	44.4	82.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	4.2994	7.28	0.00	84714	171.0	35.8	26.4	49.0




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	6.6526	12.29	-0.01	81092	122.0	14.8	9.6	17.9



Quantitation Results Report (QT Reviewed)

Data File	Dec2816.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	12/29/2021 1:07:14 AM
Sample Name	B21121613-002A	Instrument	GCMS
Vial	16	Multiplier	1.00
DA Method File		Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	122821 bna SIM 1.batch.bin	Last Calib Update	12/29/2021 8:56:55 AM

Ref Library

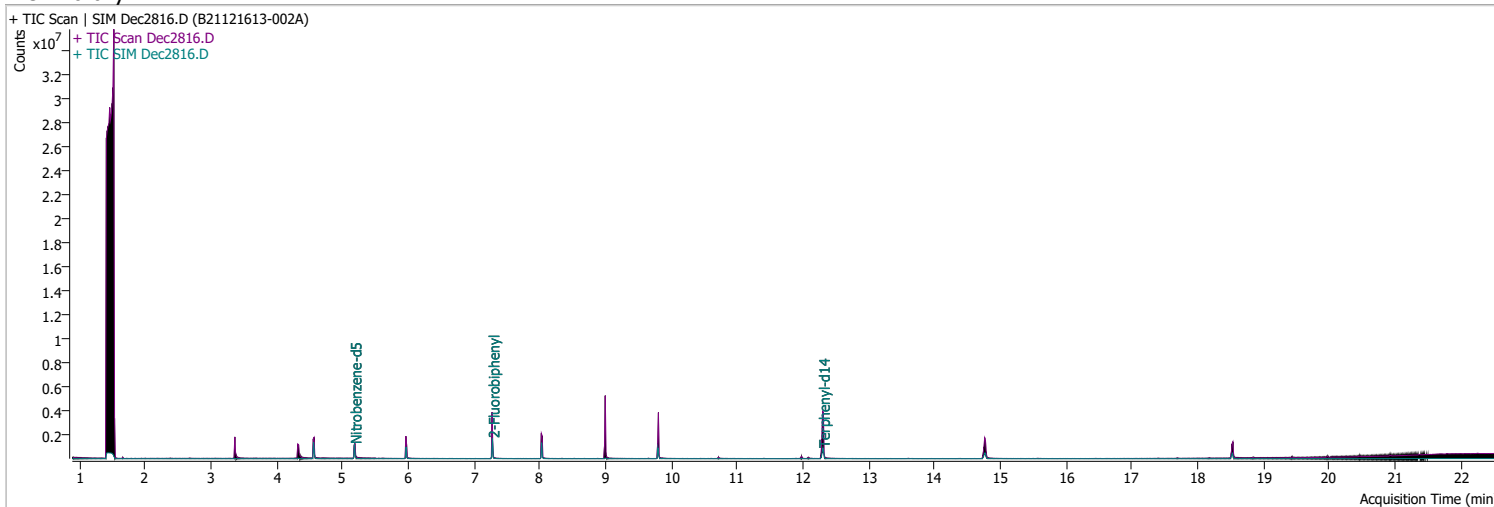

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
----------	----	------	-------	-------	-------	----------

Internal Standards

System Monitoring Compounds

S Nitrobenzene-d5	5.180	82.0	720920	38.9462	ng/ml	-0.013
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 778.92%		*
S 2-Fluorobiphenyl	7.277	172.0	1047690	48.5597	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 971.19%		*
S Terphenyl-d14	12.300	244.0	1255813	94.8449	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 1896.90%		*


Target Compounds

Target Compounds	RT	QIon	Resp.	Conc.	Units	QValue
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	38.9462	5.18	-0.01	720920	54.0	31.2	21.6	40.2
					128.0	28.1	21.3	39.5

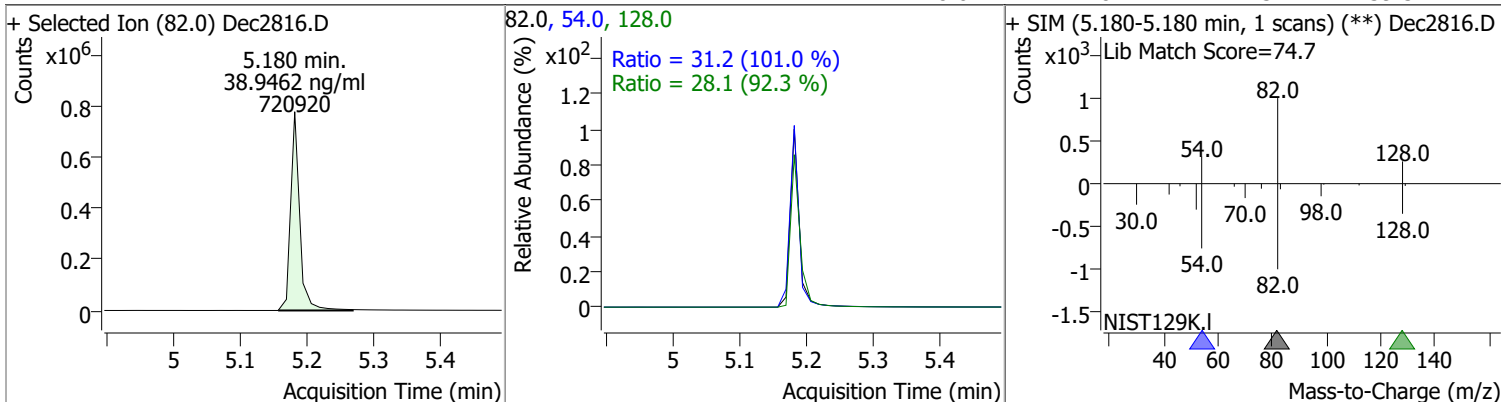


Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.99	102.0	15.5	129.0	10.8

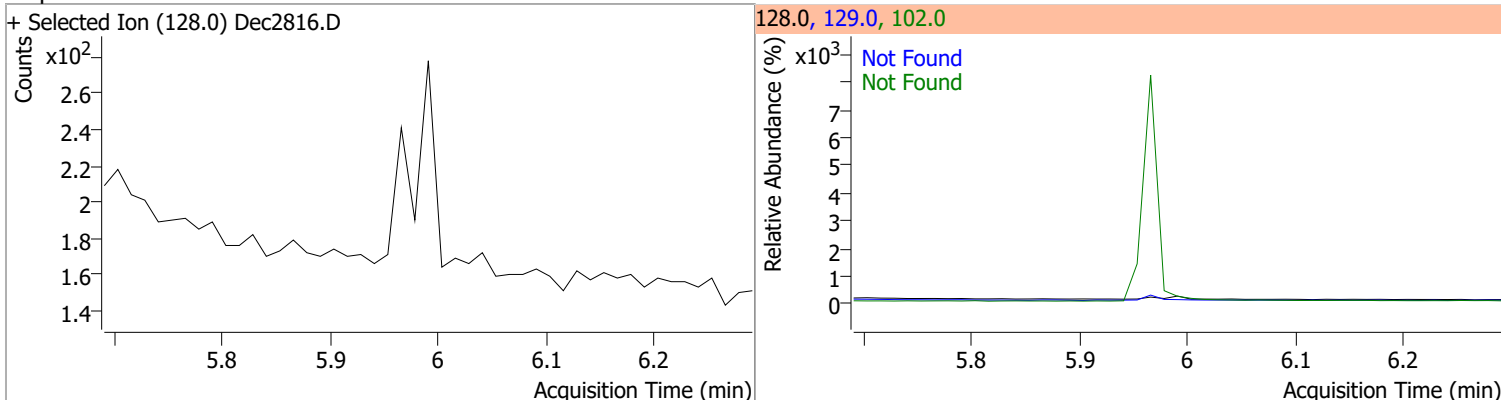

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.81	142.0	147.5	115.0	52.5



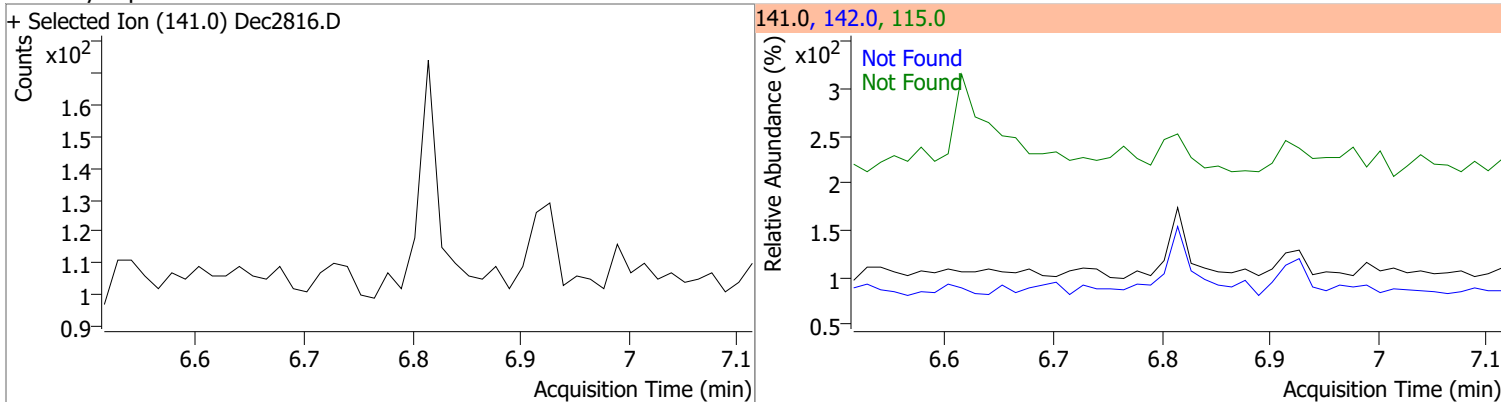


Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.93	142.0	111.3	115.0	63.4



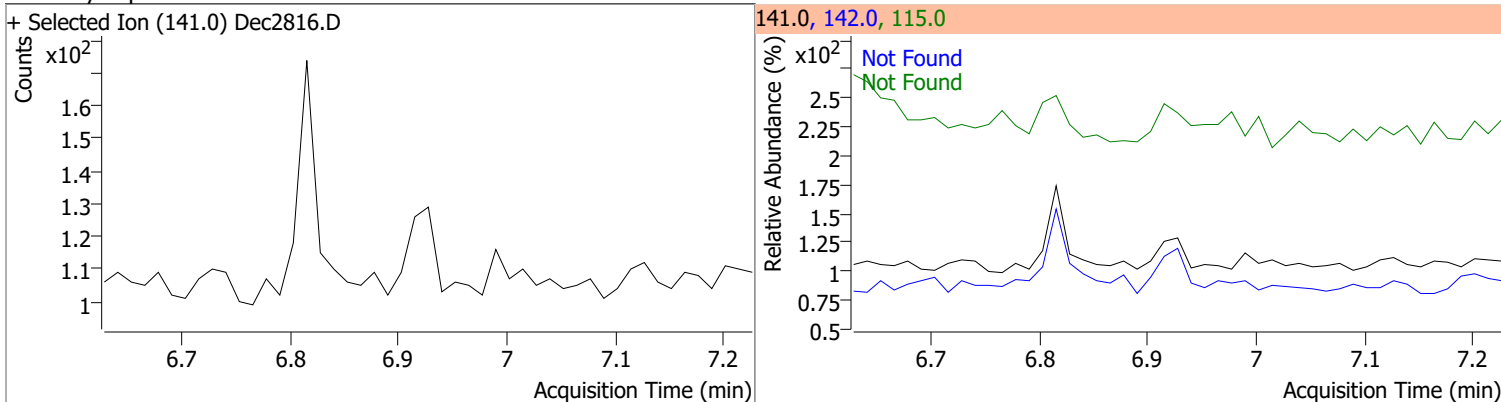


Quantitation Results Report (QT Reviewed)

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	48.5597	7.28	0.00	1047690	171.0	39.8	26.4	49.0




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	94.8449	12.30	0.00	1255813	122.0	14.6	9.6	17.9



Quantitation Results Report (QT Reviewed)

Data File	Dec2817.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	12/29/2021 1:39:59 AM
Sample Name	B21121613-002A	Instrument	GCMS
Vial	17	Multiplier	20.00
DA Method File		Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	122821 bna SIM 1.batch.bin	Last Calib Update	12/29/2021 8:56:55 AM

Ref Library

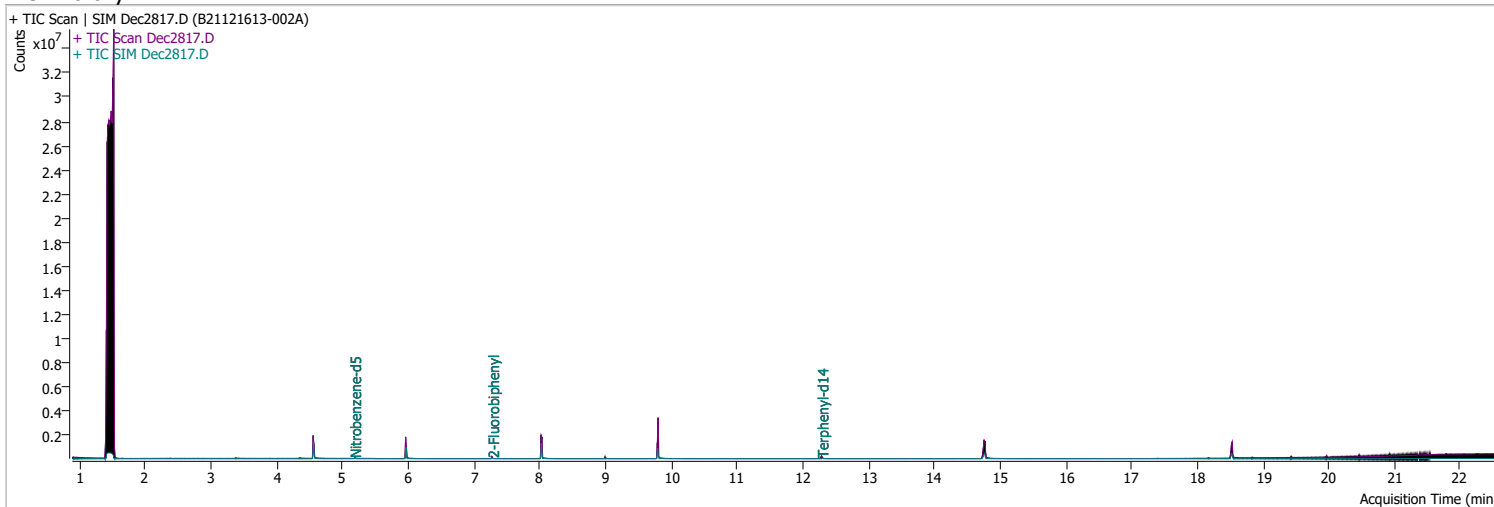

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
----------	----	------	-------	-------	-------	----------

Internal Standards

System Monitoring Compounds

S Nitrobenzene-d5	5.180	82.0	20308	44.3943	ng/ml	-0.013
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 887.89%		*
S 2-Fluorobiphenyl	7.277	172.0	56377	54.7631	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1095.26%		*
S Terphenyl-d14	12.288	244.0	56996	92.6577	ng/ml	-0.013
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 1853.15%		*


Target Compounds

Target Compounds	RT	QIon	Resp.	Conc.	Units	QValue
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	44.3943	5.18	-0.01	20308	54.0	38.1	21.6	40.2
					128.0	31.5	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.99	102.0	15.5	129.0	10.8



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.81	142.0	147.5	115.0	52.5






Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.93	142.0	111.3	115.0	63.4






Quantitation Results Report (QT Reviewed)

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	54.7631	7.28	0.00	56377	171.0	36.3	26.4	49.0

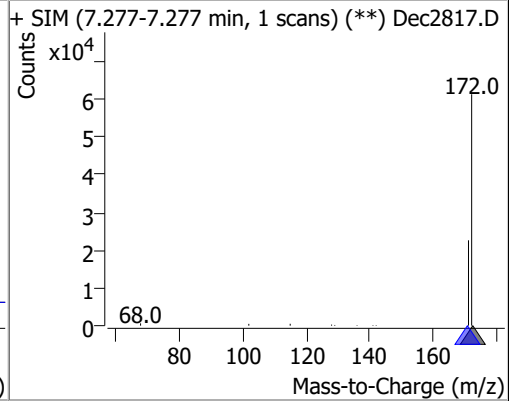


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	92.6577	12.29	-0.01	56996	122.0	14.7	9.6	17.9

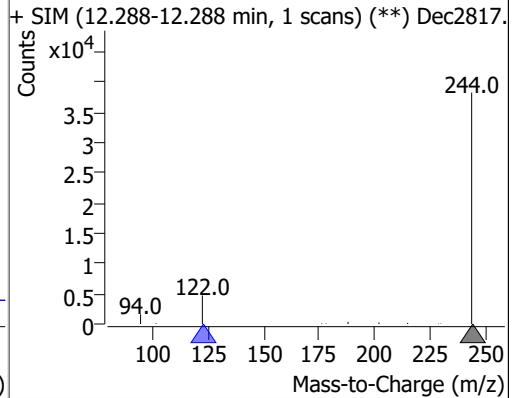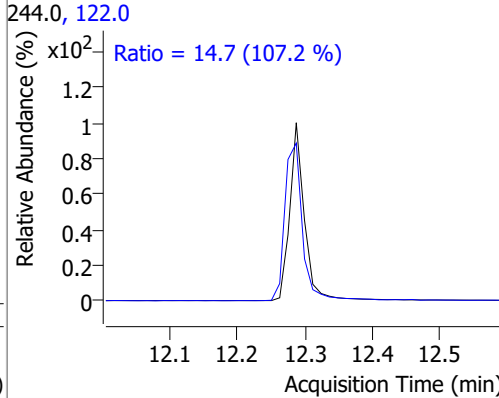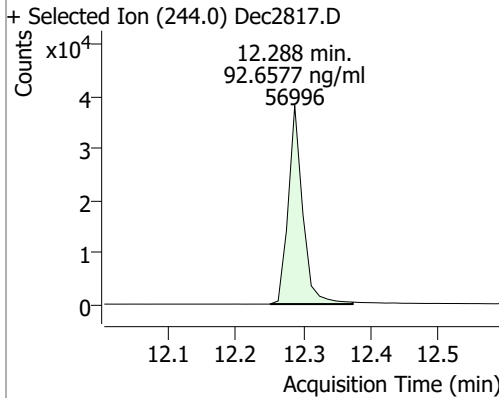

Quantitation Results Report (QT Reviewed)

Data File	Dec2818.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	12/29/2021 2:12:33 AM
Sample Name	B21121616-001B	Instrument	GCMS
Vial	18	Multiplier	1.00
DA Method File		Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	122821 bna SIM 1.batch.bin	Last Calib Update	12/29/2021 8:56:55 AM

Ref Library

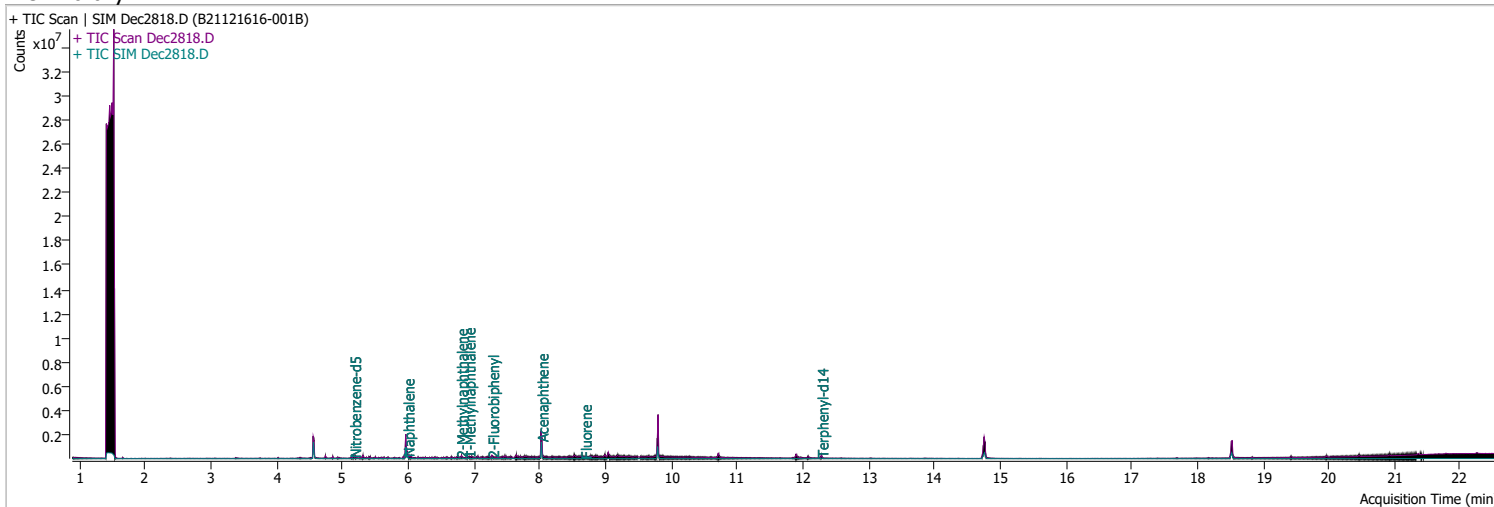

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
----------	----	------	-------	-------	-------	----------

Internal Standards

System Monitoring Compounds

S Nitrobenzene-d5	5.180	82.0	19772	2.1263	ng/ml	#	-0.013
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 42.53%			
S 2-Fluorobiphenyl	7.277	172.0	54449	2.4362	ng/ml		0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 48.72%			
S Terphenyl-d14	12.288	244.0	54916	4.0672	ng/ml		-0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 81.34%			




Target Compounds

Compound	RT	QIon	Resp.	Conc.	Units	QValue
T Naphthalene	5.991	128.0	121070	4.8105	ng/ml	m 96
T 2-Methylnaphthalene	6.802	141.0	13804	0.9510	ng/ml	# 59
T 1-Methylnaphthalene	6.915	141.0	29628	2.2075	ng/ml	97




(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	2.1263	5.18	-0.01	19772	54.0	38.3	21.6	40.2
					128.0	44.1	21.3	39.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	4.8105	5.99	0.00	121070 (m)	102.0	17.4	0.0	46.6
					129.0	11.8	7.6	14.1




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	0.9510	6.80	-0.01	13804	142.0	152.5	103.3	191.8
					115.0	154.3	36.8	68.3




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	2.2075	6.91	-0.01	29628	142.0	109.4	77.9	144.7
					115.0	66.4	44.4	82.5

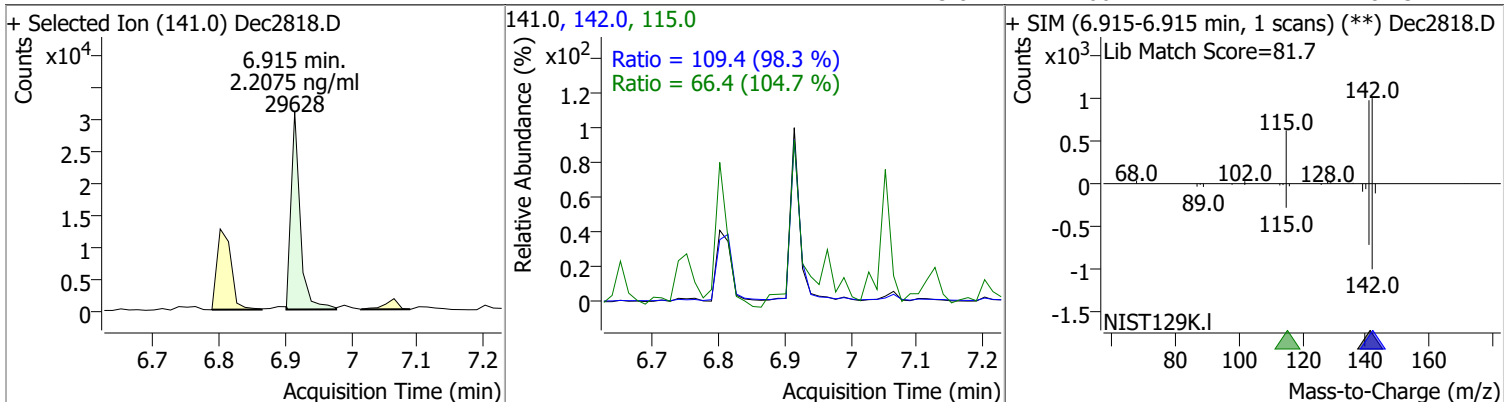

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	2.4362	7.28	0.00	54449	171.0	35.6	26.4	49.0

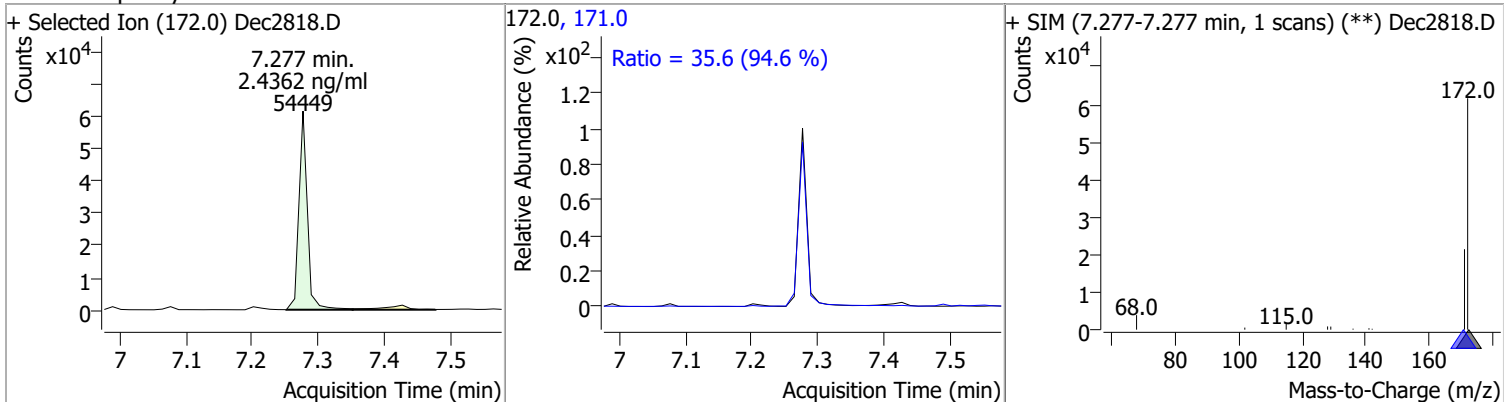


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	4.0672	12.29	-0.01	54916	122.0	14.6	9.6	17.9



Quantitation Results Report (QT Reviewed)

Data File	Dec2819.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	12/29/2021 2:45:08 AM
Sample Name	B21121622-001A	Instrument	GCMS
Vial	19	Multiplier	1.00
DA Method File		Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	122821 bna SIM 1.batch.bin	Last Calib Update	12/29/2021 8:56:55 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
----------	----	------	-------	-------	-------	----------

Internal Standards

System Monitoring Compounds

S Nitrobenzene-d5	5.180	82.0	35685	3.7623	ng/ml	-0.013
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 75.25%		
S 2-Fluorobiphenyl	7.277	172.0	66056	3.1477	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 62.95%		
S Terphenyl-d14	12.288	244.0	54726	3.9153	ng/ml	-0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 78.31%		


Target Compounds

Target Compounds	RT	QIon	Resp.	Conc.	Units	QValue
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	3.7623	5.18	-0.01	35685	54.0	29.9	21.6	40.2
					128.0	27.6	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.99	102.0	15.5	129.0	10.8



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.81	142.0	147.5	115.0	52.5






Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.93	142.0	111.3	115.0	63.4






Quantitation Results Report (QT Reviewed)

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	3.1477	7.28	0.00	66056	171.0	35.5	26.4	49.0




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	3.9153	12.29	-0.01	54726	122.0	14.3	9.6	17.9



Quantitation Results Report (QT Reviewed)

Data File	Dec2820.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	12/29/2021 3:17:40 AM
Sample Name	B21121622-002A	Instrument	GCMS
Vial	20	Multiplier	1.00
DA Method File		Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	122821 bna SIM 1.batch.bin	Last Calib Update	12/29/2021 8:56:55 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
----------	----	------	-------	-------	-------	----------

Internal Standards

System Monitoring Compounds

S Nitrobenzene-d5	5.180	82.0	32932	3.6422	ng/ml	-0.013
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 72.84%		
S 2-Fluorobiphenyl	7.277	172.0	64961	3.2477	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 64.95%		
S Terphenyl-d14	12.288	244.0	51797	4.6504	ng/ml	-0.013
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 93.01%		


Target Compounds

Target Compounds	RT	QIon	Resp.	Conc.	Units	QValue
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	3.6422	5.18	-0.01	32932	54.0	29.8	21.6	40.2
					128.0	27.3	21.3	39.5

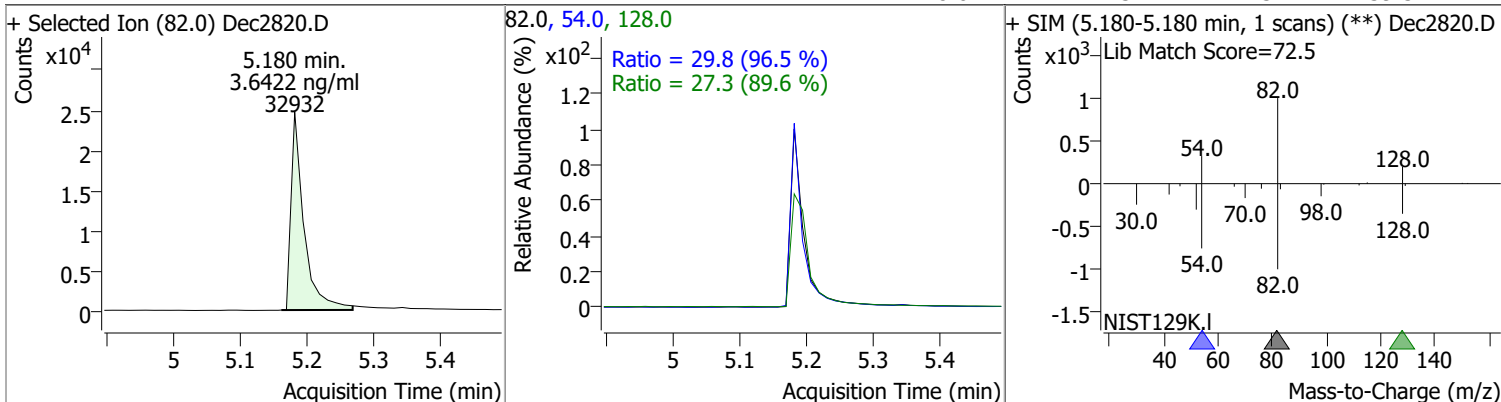


Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.99	102.0	15.5	129.0	10.8

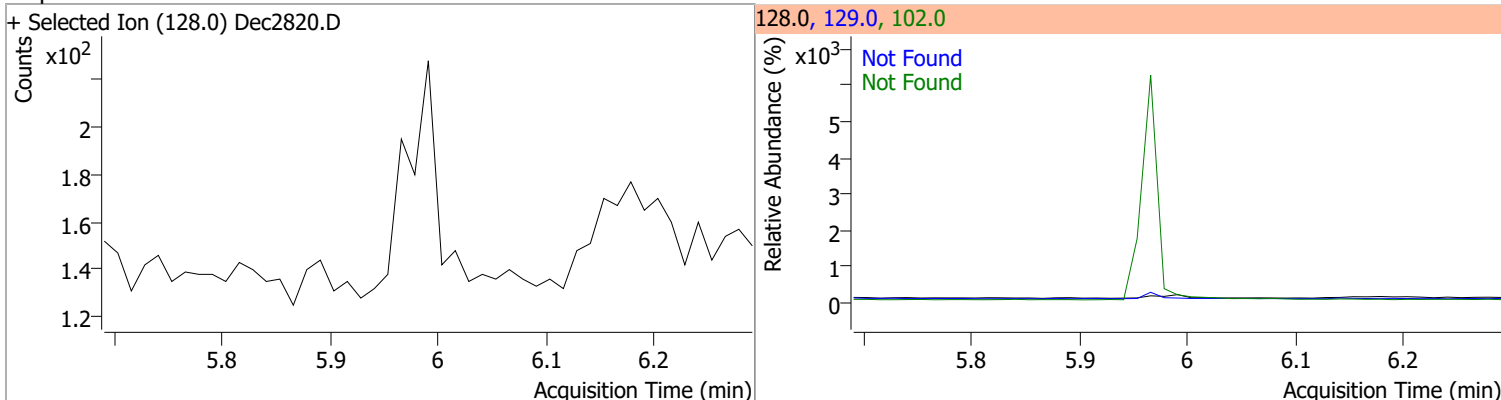

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.81	142.0	147.5	115.0	52.5



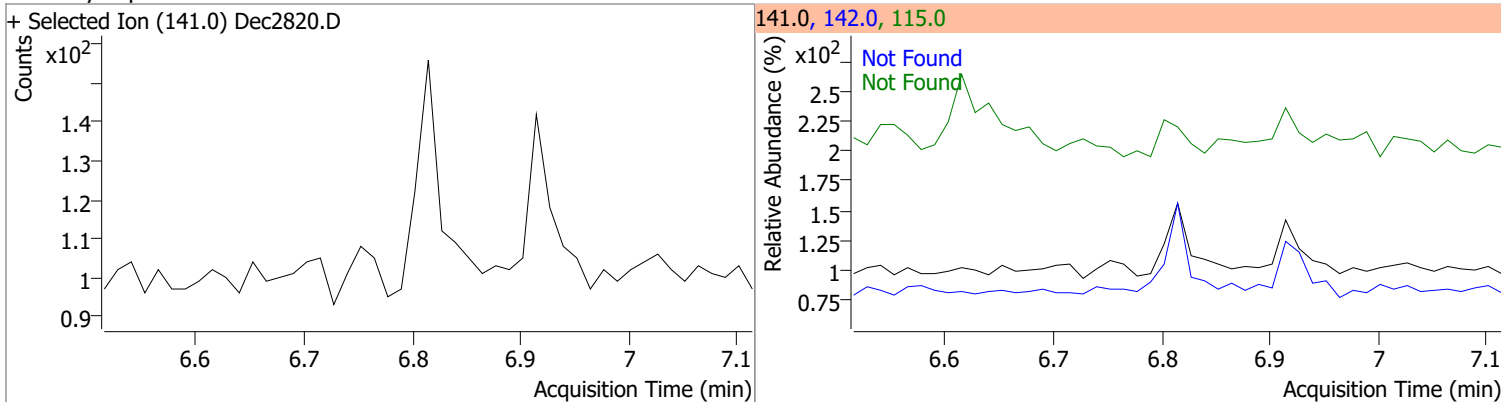


Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.93	142.0	111.3	115.0	63.4



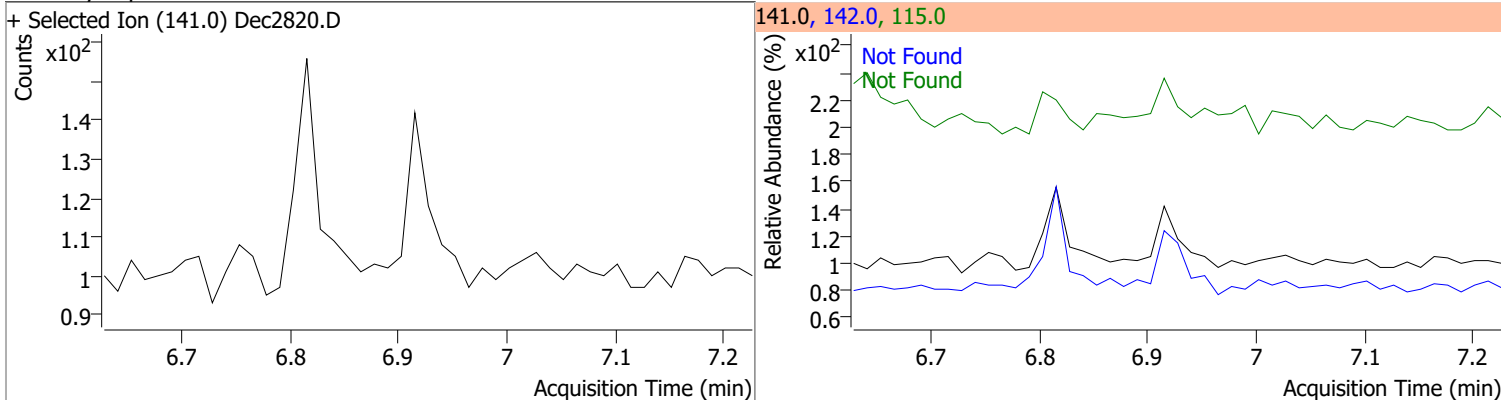


Quantitation Results Report (QT Reviewed)

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	3.2477	7.28	0.00	64961	171.0	35.0	26.4	49.0




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	4.6504	12.29	-0.01	51797	122.0	15.2	9.6	17.9



Quantitation Results Report (QT Reviewed)

Data File	Dec2821.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	12/29/2021 3:50:36 AM
Sample Name	B21121622-003A	Instrument	GCMS
Vial	21	Multiplier	1.00
DA Method File		Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	122821 bna SIM 1.batch.bin	Last Calib Update	12/29/2021 8:56:55 AM

Ref Library

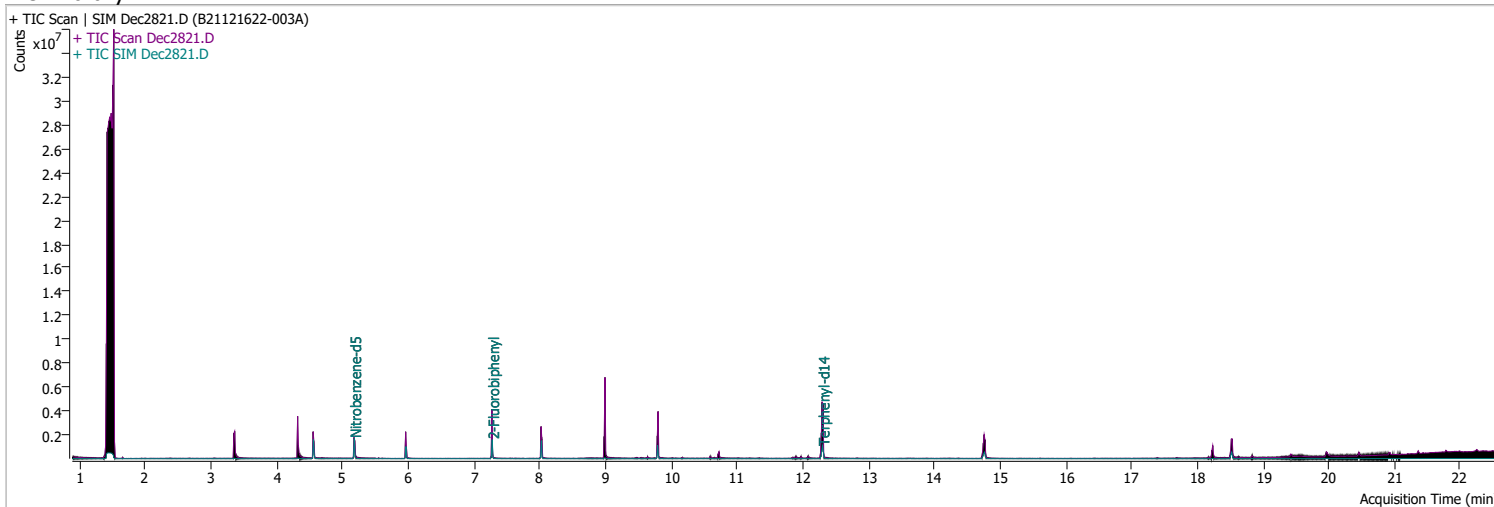

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
----------	----	------	-------	-------	-------	----------

Internal Standards

System Monitoring Compounds

S Nitrobenzene-d5	5.180	82.0	985912	45.6744	ng/ml	-0.013
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 913.49%		*
S 2-Fluorobiphenyl	7.277	172.0	994439	41.2036	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 824.07%		*
S Terphenyl-d14	12.300	244.0	1556131	102.5060	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 2050.12%		*


Target Compounds

T Naphthalene	0.000		0	N.D.		QValue
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	45.6744	5.18	-0.01	985912	54.0	33.6	21.6	40.2
					128.0	28.2	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.99	102.0	15.5	129.0	10.8



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.81	142.0	147.5	115.0	52.5






Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.93	142.0	111.3	115.0	63.4



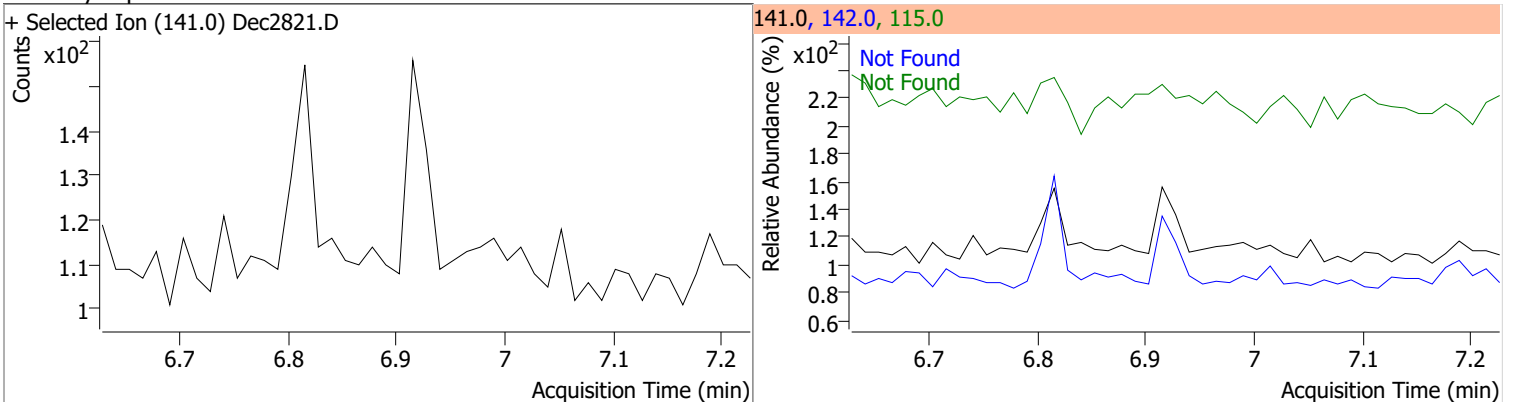


Quantitation Results Report (QT Reviewed)

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	41.2036	7.28	0.00	994439	171.0	39.2	26.4	49.0




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	102.5060	12.30	0.00	1556131	122.0	14.3	9.6	17.9



Quantitation Results Report (QT Reviewed)

Data File	Dec2822.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	12/29/2021 4:23:11 AM
Sample Name	B21121622-003A	Instrument	GCMS
Vial	22	Multiplier	20.00
DA Method File		Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	122821 bna SIM 1.batch.bin	Last Calib Update	12/29/2021 8:56:55 AM

Ref Library

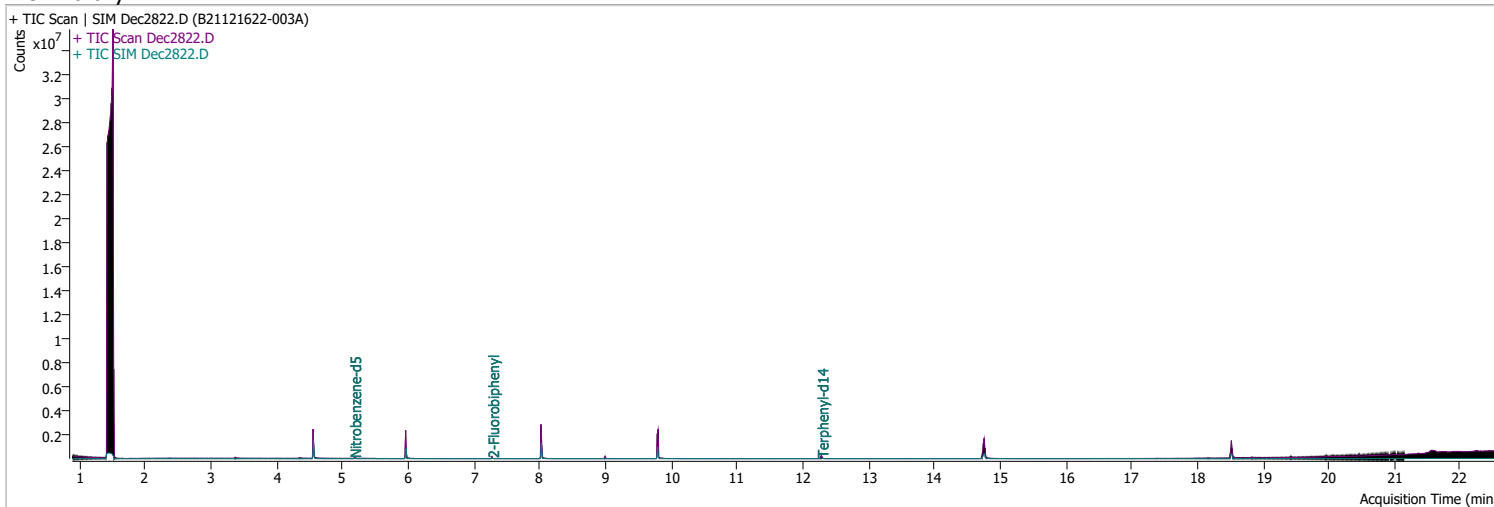

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
----------	----	------	-------	-------	-------	----------

Internal Standards

System Monitoring Compounds

S Nitrobenzene-d5	5.181	82.0	33275	68.5555	ng/ml	-0.012
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 1371.11%		*
S 2-Fluorobiphenyl	7.277	172.0	47634	44.9096	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 898.19%		*
S Terphenyl-d14	12.288	244.0	62560	100.7769	ng/ml	-0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 2015.54%		*


Target Compounds

Target Compounds	RT	QIon	Resp.	Conc.	Units	QValue
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	68.5555	5.18	-0.01	33275	54.0	28.7	21.6	40.2
					128.0	21.6	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.99	102.0	15.5	129.0	10.8



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.81	142.0	147.5	115.0	52.5






Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.93	142.0	111.3	115.0	63.4






Quantitation Results Report (QT Reviewed)

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	44.9096	7.28	0.00	47634	171.0	35.5	26.4	49.0

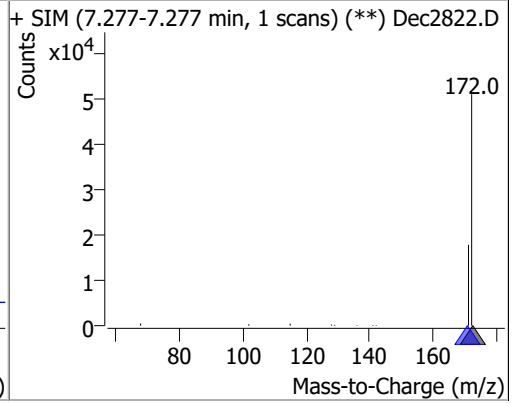


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	100.7769	12.29	-0.01	62560	122.0	14.8	9.6	17.9

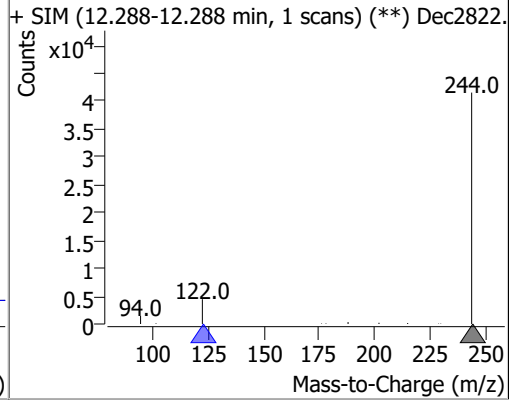

Quantitation Results Report (QT Reviewed)

Data File	Dec2823.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	12/29/2021 4:55:51 AM
Sample Name	B21121623-001B	Instrument	GCMS
Vial	23	Multiplier	1.00
DA Method File		Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	122821 bna SIM 1.batch.bin	Last Calib Update	12/29/2021 8:56:55 AM

Ref Library

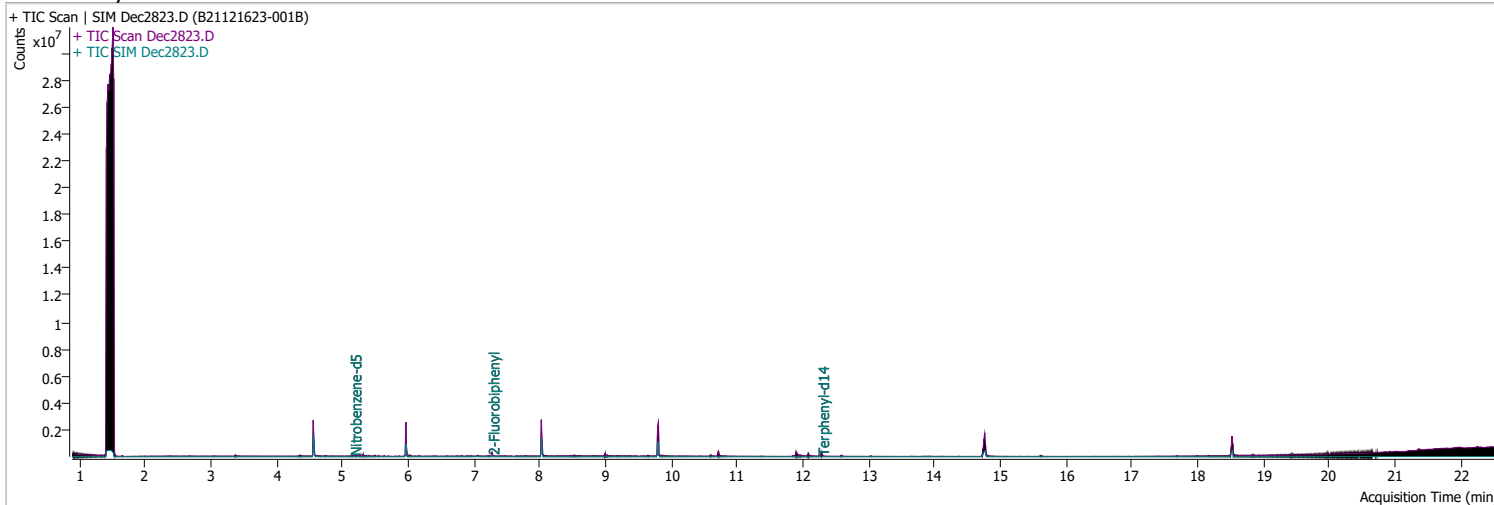


Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
System Monitoring Compounds						
S Nitrobenzene-d5	5.181	82.0	39500	3.6233	ng/ml #	-0.012
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 72.47%		
S 2-Fluorobiphenyl	7.277	172.0	76083	3.2838	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 65.68%		
S Terphenyl-d14	12.288	244.0	64933	5.0373	ng/ml	-0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 100.75%		
Target Compounds						
T Naphthalene	6.003	128.0	0		ng/ml md	1
T 2-Methylnaphthalene	7.065	141.0	0		ng/ml md	1
T 1-Methylnaphthalene	7.065	141.0	0		ng/ml md	1


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	3.6233	5.18	-0.01	39500	54.0	29.6	21.6	40.2
					128.0	19.3	21.3	39.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	0	0	0	0	102.0	0.0	0.0	46.6
					129.0	7.6	7.6	14.1




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	0	0	0	0	142.0	103.3	103.3	191.8
					115.0	36.8	36.8	68.3




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene		0		0	142.0		77.9	144.7
					115.0		44.4	82.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	3.2838	7.28	0.00	76083	171.0	35.0	26.4	49.0




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	5.0373	12.29	-0.01	64933	122.0	14.4	9.6	17.9



Quantitation Results Report (QT Reviewed)

Data File	Dec2824.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	12/29/2021 5:28:26 AM
Sample Name	28-Dec-21_CCV_24	Instrument	GCMS
Vial	24	Multiplier	1.00
DA Method File		Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	122821 bna SIM 1.batch.bin	Last Calib Update	12/29/2021 8:56:55 AM

Ref Library

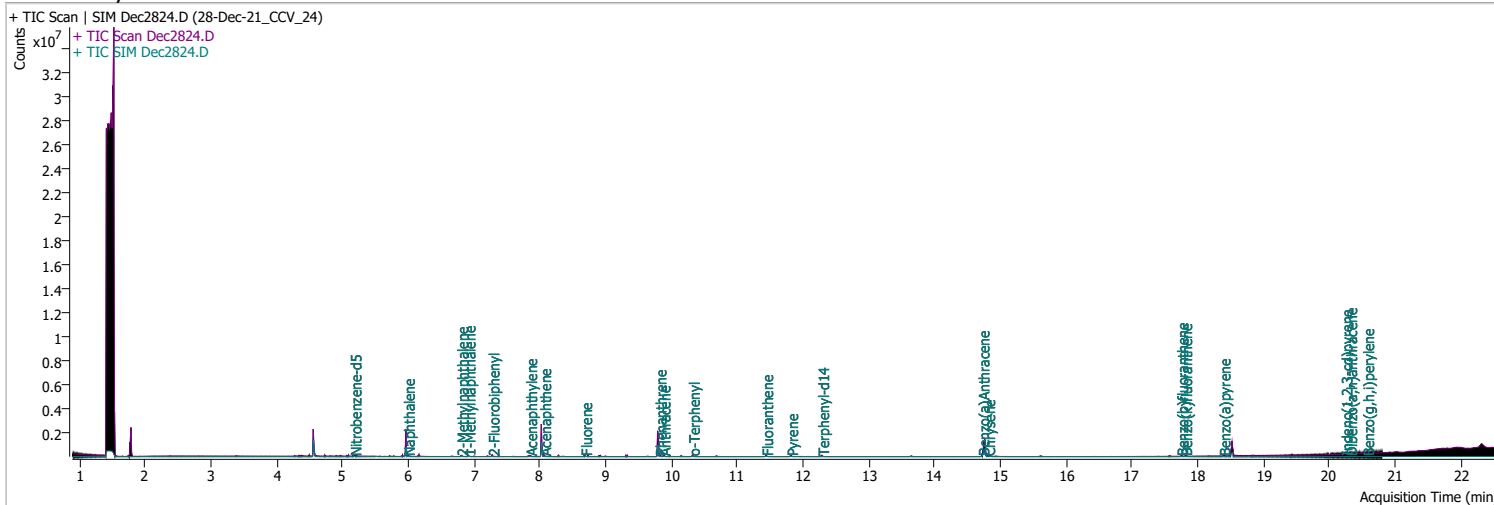

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
----------	----	------	-------	-------	-------	----------

Internal Standards

System Monitoring Compounds

S Nitrobenzene-d5	5.181	82.0	18436	2.1087	ng/ml	-0.012
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 42.17%		
S 2-Fluorobiphenyl	7.277	172.0	34193	1.7070	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 34.14%		
S Terphenyl-d14	12.288	244.0	20472	1.8499	ng/ml	-0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 37.00%		*




Target Compounds

Compound	RT	QIon	Resp.	Conc.	Units	QValue
T Naphthalene	5.991	128.0	36414	1.5686	ng/ml	80
T 2-Methylnaphthalene	6.802	141.0	24142	1.8033	ng/ml	91
T 1-Methylnaphthalene	6.915	141.0	25483	2.0585	ng/ml	95




(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	2.1087	5.18	-0.01	18436	54.0	30.9	21.6	40.2
					128.0	28.1	21.3	39.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	1.5686	5.99	0.00	36414	102.0	29.3	0.0	46.6
					129.0	11.0	7.6	14.1




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	1.8033	6.80	-0.01	24142	142.0	138.7	103.3	191.8
					115.0	62.2	36.8	68.3




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	2.0585	6.91	-0.01	25483	142.0	112.5	77.9	144.7
					115.0	54.2	44.4	82.5

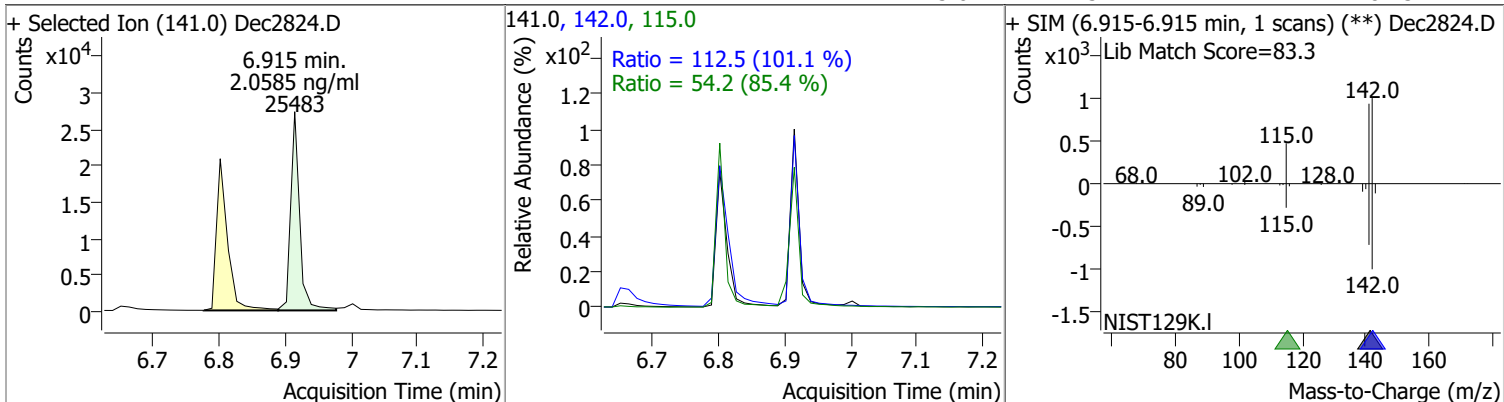

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	1.7070	7.28	0.00	34193	171.0	33.0	26.4	49.0

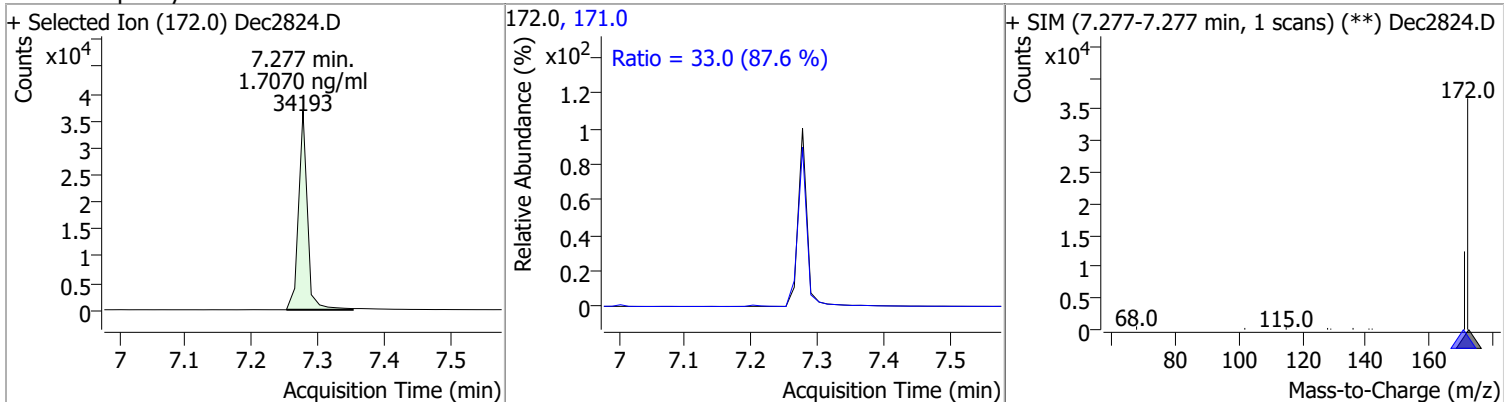

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	1.8499	12.29	-0.01	20472	122.0	14.9	9.6	17.9



Audit Trail report

Batch name and path: \\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\QuantResults\122821 bna SIM 1.batch.bin
Quant batch version: 10.0
Quant reporting version: 10.0

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdNewBatchTable	BL2000\jheine	12/28/2021 12:35:55 PM	Create new batch \\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\122821 bna SIM 1.batch.bin			✓	
CmdImportSamplesFromWorklist	BL2000\jheine	12/28/2021 12:35:59 PM	Add samples from worklist: \\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2801.D			✓	
CmdSetSampleAttribute	BL2000\jheine	12/28/2021 12:36:03 PM	Set SampleType = TuneCheck for sample Dec2801.D; previous value = Sample			✓	
CmdSaveBatchTable	BL2000\jheine	12/28/2021 1:35:28 PM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\QuantResults\122821 bna SIM 1.batch.bin			✓	
CmdOpenBatchTable	BL2000\jheine	12/29/2021 8:03:39 AM	Open batch \\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\122821 bna SIM 1.batch.bin			✓	
CmdRemoveSamples	BL2000\jheine	12/29/2021 8:03:52 AM	Remove 1 sample(s): Remove TuneCheck sample 28-Dec-21_TUNE_1, data file Dec2801.D ;			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdImportSamplesFromWorklist	BL2000\jheine	12/29/2021 8:05:00 AM	Add samples from worklist: \\MASSHUNTER\Org\Data\SV5975.I\sh 122821\1 e8270c bna SIM\Dec2824.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 122821\1 e8270c bna SIM\Dec2823.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 122821\1 e8270c bna SIM\Dec2822.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 122821\1 e8270c bna SIM\Dec2821.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 122821\1 e8270c bna SIM\Dec2820.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 122821\1 e8270c bna SIM\Dec2819.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 122821\1 e8270c bna SIM\Dec2818.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 122821\1 e8270c bna SIM\Dec2817.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 122821\1 e8270c bna SIM\Dec2816.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 122821\1 e8270c bna SIM\Dec2815.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 122821\1 e8270c bna SIM\Dec2814.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 122821\1 e8270c bna SIM\Dec2813.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 122821\1 e8270c bna SIM\Dec2812.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 122821\1 e8270c bna SIM\Dec2811.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 122821\1 e8270c bna SIM\Dec2810.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 122821\1 e8270c bna SIM\Dec2809.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 122821\1 e8270c bna SIM\Dec2808.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 122821\1 e8270c bna SIM\Dec2807.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 122821\1 e8270c bna SIM\Dec2806.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 122821\1 e8270c bna SIM\Dec2805.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 122821\1 e8270c bna SIM\Dec2804.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 122821\1 e8270c bna SIM\Dec2803.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 122821\1 e8270c bna SIM\Dec2802.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 122821\1 e8270c bna SIM\Dec2801.D			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 8:16:09 AM	Set SampleType = TuneCheck for sample Dec2801.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 8:16:54 AM	Set SampleType = Calibration for sample Dec2802.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 8:16:57 AM	Set SampleType = Calibration for sample Dec2803.D; previous value = Sample			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 8:16:59 AM	Set SampleType = Calibration for sample Dec2804.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 8:17:01 AM	Set SampleType = Calibration for sample Dec2805.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 8:17:03 AM	Set SampleType = Calibration for sample Dec2806.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 8:17:05 AM	Set SampleType = Calibration for sample Dec2807.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 8:17:08 AM	Set SampleType = Calibration for sample Dec2808.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 8:17:12 AM	Set SampleType = QC for sample Dec2809.D; previous value = Sample			✓	
CmdStartMethodEditing	BL2000\jheine	12/29/2021 8:17:33 AM	Start method editing			✓	
CmdImportMethodFromBatch	BL2000\jheine	12/29/2021 8:17:35 AM	Import method from batch \\MASSHUNTER\Org\Data\SV5975.I\sh 122721\1 e8270c bna SIM\122721 bna SIM 1.batch.bin			✓	
CmdApplyMethodToAllSamples	BL2000\jheine	12/29/2021 8:17:42 AM	Apply method to all samples			✓	
CmdMethodClear	BL2000\jheine	12/29/2021 8:17:42 AM	Clear method			✓	
CmdEndMethodEditing	BL2000\jheine	12/29/2021 8:17:43 AM	End method editing			✓	
CmdQuantitate	BL2000\jheine	12/29/2021 8:17:55 AM	Quantitate all compounds in all samples			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 8:18:19 AM	Set LevelName = 7 for sample Dec2802.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 8:18:28 AM	Set LevelName = 6 for sample Dec2803.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 8:18:40 AM	Set LevelName = 5 for sample Dec2804.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 8:18:49 AM	Set LevelName = 4 for sample Dec2805.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 8:18:57 AM	Set LevelName = 3 for sample Dec2806.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 8:19:06 AM	Set LevelName = 2 for sample Dec2807.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 8:19:15 AM	Set LevelName = 1 for sample Dec2808.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 8:19:25 AM	Set LevelName = ICV for sample Dec2809.D; previous value =			✓	
CmdQuantitate	BL2000\jheine	12/29/2021 8:19:41 AM	Quantitate all compounds in all samples			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 8:20:14 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Dec2804.D, from x, y = 5.978, 534 to 6.116, 103, result = 4116; previous integration is from x, y = 5.941, 103 to 6.116, 103 and previous response = 11635.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 8:20:16 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Dec2804.D to y = 103, new integration is from x, y = 5.978, 103 to 6.116, 103 and new response = 5894; previous integration is from x, y = 5.978, 534 to 6.116, 103 and previous response = 4116.			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	12/29/2021 8:20:23 AM	Split peak for compound 2-Methylnaphthalene in sample Dec2804.D and keep left peak, new integration is from x, y = 6.790, 119.732142857143 to 6.902, 119.732142857143 and new response = 21520, previous integration is from x, y = 6.790, 120 to 6.990, 120 and previous response = 41032.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:20:26 AM	Set UserAnnotation = CO for compound 2-Methylnaphthalene in sample Dec2804.D; previous value =			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	12/29/2021 8:20:30 AM	Split peak for compound 1-Methylnaphthalene in sample Dec2804.D and keep right peak, new integration is from x, y = 6.902, 119.732142857143 to 6.990, 119.732142857143 and new response = 19512, previous integration is from x, y = 6.790, 120 to 6.990, 120 and previous response = 41032.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:20:32 AM	Set UserAnnotation = CO for compound 1-Methylnaphthalene in sample Dec2804.D; previous value =			✓	
CmdSelectPeak	BL2000\jheine	12/29/2021 8:20:46 AM	Select peak for compound Phenanthrene in sample Dec2804.D			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:20:48 AM	Set UserAnnotation = RT for compound Phenanthrene in sample Dec2804.D; previous value =			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	12/29/2021 8:21:00 AM	Split qualifier 101.0 of compound Fluoranthene in sample Dec2804.D and keep left peak, new integration is from x, y = 11.412, 77.20875 to 11.559, 77.20875 and new response = 5107, previous integration is from x, y = 11.412, 77 to 11.954, 77 and previous response = 12100.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateSplit	BL2000\jheine	12/29/2021 8:21:10 AM	Split qualifier 101.0 of compound Pyrene in sample Dec2804.D and keep right peak, new integration is from x, y = 11.769, 77.20875 to 11.954, 77.20875 and new response = 6822, previous integration is from x, y = 11.412, 77 to 11.954, 77 and previous response = 12100.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	12/29/2021 8:21:18 AM	Manually integrate compound Benzo(a)Anthracene in sample Dec2804.D, from x, y = 14.739, 3882 to 14.739, 3704, result = 0; previous integration is from x, y = 14.801, 61 to 15.000, 62 and previous response = 43320.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:21:20 AM	Set UserAnnotation = RT for compound Benzo(a)Anthracene in sample Dec2804.D; previous value =			✓	
CmdClearManualIntegration	BL2000\jheine	12/29/2021 8:21:26 AM	Clear manual integration of target signal for compound Benzo(a)Anthracene in sample Dec2804.D			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:21:27 AM	Set UserAnnotation = for compound Benzo(a)Anthracene in sample Dec2804.D; previous value = RT			✓	
CmdSelectPeak	BL2000\jheine	12/29/2021 8:21:29 AM	Select peak for compound Benzo(a)Anthracene in sample Dec2804.D			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:21:32 AM	Set UserAnnotation = RT for compound Benzo(a)Anthracene in sample Dec2804.D; previous value =			✓	
CmdSelectPeak	BL2000\jheine	12/29/2021 8:21:39 AM	Select peak for compound Benzo(b)fluoranthene in sample Dec2804.D			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:21:42 AM	Set UserAnnotation = RT for compound Benzo(b)fluoranthene in sample Dec2804.D; previous value =			✓	
CmdSelectPeak	BL2000\jheine	12/29/2021 8:21:49 AM	Select peak for compound Indeno(1,2,3-cd)pyrene in sample Dec2804.D			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:21:52 AM	Set UserAnnotation = RT for compound Indeno(1,2,3-cd)pyrene in sample Dec2804.D; previous value =			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdUpdateRetentionTimes	BL2000\jheine	12/29/2021 8:22:08 AM	Update retention time for compound Perylene-d12; Chrysene-d12; Phenanthrene-d10; Acenaphthene-d10; Naphthalene-d8; 1,4-Dichlorobenzene-d4; o-Terphenyl; Terphenyl-d14; 2-Fluorobiphenyl; Nitrobenzene-d5; Dibenzo(a,h)anthracene; Indeno(1,2,3-cd)pyrene; Benzo(a)pyrene; Benzo(k)fluoranthene; Benzo(b)fluoranthene; Chrysene; Benzo(a)Anthracene; Pyrene; Fluoranthene; Anthracene; Phenanthrene; Fluorene; Acenaphthene; Acenaphthylene; 1-Methylnaphthalene; 2-Methylnaphthalene; Naphthalene; Benzo(g,h,i)perylene;			✓	
CmdQuantitate	BL2000\jheine	12/29/2021 8:22:23 AM	Quantitate all compounds in all samples			✓	
CmdQuantitate	BL2000\jheine	12/29/2021 8:23:25 AM	Quantitate all compounds in all samples			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 8:23:43 AM	Manually integrate qualifier 54.0 of compound Nitrobenzene-d5 in sample Dec2804.D, from x, y = 5.168, 487 to 5.280, 207, result = 3432; previous integration is from x, y = 5.131, 209 to 5.280, 207 and previous response = 4500.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 8:23:45 AM	Drop baseline for qualifier 54.0 of compound Nitrobenzene-d5 in sample Dec2804.D to y = 207, new integration is from x, y = 5.168, 207 to 5.280, 207 and new response = 4373; previous integration is from x, y = 5.168, 487 to 5.280, 207 and previous response = 3432.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdUpdateQualifierRatios	BL2000\jheine	12/29/2021 8:24:41 AM	Update qualifier ratios for compound Perylene-d12; Update qualifier ratios for compound Chrysene-d12; Update qualifier ratios for compound Phenanthrene-d10; Update qualifier ratios for compound Acenaphthene-d10; Update qualifier ratios for compound Naphthalene-d8; Update qualifier ratios for compound 1,4-Dichlorobenzene-d4; Update qualifier ratios for compound o-Terphenyl; Update qualifier ratios for compound Terphenyl-d14; Update qualifier ratios for compound 2-Fluorobiphenyl; Update qualifier ratios for compound Benzo(g,h,i)perylene; Update qualifier ratios for compound Dibenzo(a,h)anthracene; Update qualifier ratios for compound Indeno(1,2,3-cd)pyrene; Update qualifier ratios for compound Benzo(a)pyrene; Update qualifier ratios for compound Benzo(k)fluoranthene; Update qualifier ratios for compound Benzo(b)fluoranthene; Update qualifier ratios for compound Chrysene; Update qualifier ratios for compound Benzo(a)Anthracene; Update qualifier ratios for compound Pyrene; Update qualifier ratios for compound Fluoranthene; Update qualifier ratios for compound Anthracene; Update qualifier ratios for compound Phenanthrene; Update qualifier ratios for compound Fluorene; Update qualifier ratios for compound Acenaphthene; Update qualifier ratios for compound Acenaphthylene; Update qualifier ratios for compound 1-Methylnaphthalene; Update qualifier ratios for compound 2-Methylnaphthalene; Update qualifier ratios for compound Naphthalene; Update qualifier ratios for compound Nitrobenzene-d5;			✓	
CmdQuantitate	BL2000\jheine	12/29/2021 8:27:14 AM	Quantitate all compounds in all samples			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 8:29:50 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Dec2803.D, from x, y = 5.978, 877 to 6.078, 118, result = 11868; previous integration is from x, y = 5.941, 118 to 6.078, 118 and previous response = 20539.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 8:29:51 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Dec2803.D to y = 118, new integration is from x, y = 5.978, 118 to 6.078, 118 and new response = 14143; previous integration is from x, y = 5.978, 877 to 6.078, 118 and previous response = 11868.			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	12/29/2021 8:29:56 AM	Split peak for compound 2-Methylnaphthalene in sample Dec2803.D and keep left peak, new integration is from x, y = 6.777, 126.485615079365 to 6.902, 126.485615079365 and new response = 54126, previous integration is from x, y = 6.777, 126 to 6.990, 126 and previous response = 104540.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:29:58 AM	Set UserAnnotation = CO for compound 2-Methylnaphthalene in sample Dec2803.D; previous value =			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	12/29/2021 8:30:05 AM	Split peak for compound 1-Methylnaphthalene in sample Dec2803.D and keep right peak, new integration is from x, y = 6.902, 126.485615079365 to 6.990, 126.485615079365 and new response = 50414, previous integration is from x, y = 6.777, 126 to 6.990, 126 and previous response = 104540.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:30:08 AM	Set UserAnnotation = CO for compound 1-Methylnaphthalene in sample Dec2803.D; previous value =			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 8:30:49 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Dec2805.D, from x, y = 5.978, 475 to 6.053, 98, result = 2389; previous integration is from x, y = 5.921, 98 to 6.053, 98 and previous response = 8522.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 8:30:51 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Dec2805.D to y = 98, new integration is from x, y = 5.978, 98 to 6.053, 98 and new response = 3238; previous integration is from x, y = 5.978, 475 to 6.053, 98 and previous response = 2389.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 8:31:05 AM	Manually integrate qualifier 167.0 of compound Fluorene in sample Dec2805.D, from x, y = 8.673, 251 to 8.723, 476, result = 959; previous integration is from x, y = 8.885, 98 to 8.985, 98 and previous response = 2823.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	12/29/2021 8:31:07 AM	Snap baseline for qualifier 167.0 of compound Fluorene in sample Dec2805.D from x = 8.673 to x = 8.723, new integration is from x, y = 8.673, 97 to 8.723, 165 and new response = 1654; previous integration is from x, y = 8.673, 251 to 8.723, 476 and previous response = 959.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 8:31:08 AM	Drop baseline for qualifier 167.0 of compound Fluorene in sample Dec2805.D to y = 97, new integration is from x, y = 8.673, 97 to 8.723, 97 and new response = 1756; previous integration is from x, y = 8.673, 97 to 8.723, 165 and previous response = 1654.			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	12/29/2021 8:31:14 AM	Split peak for compound Phenanthrene in sample Dec2805.D and keep left peak, new integration is from x, y = 9.780, 92.9087593565855 to 9.867, 92.9087593565855 and new response = 21524, previous integration is from x, y = 9.780, 93 to 9.916, 93 and previous response = 38338.			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	12/29/2021 8:31:17 AM	Split qualifier 176.0 of compound Phenanthrene in sample Dec2805.D and keep left peak, new integration is from x, y = 9.780, 69.237035002035 to 9.867, 69.237035002035 and new response = 4018, previous integration is from x, y = 9.780, 69 to 9.916, 69 and previous response = 7091.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:31:23 AM	Set UserAnnotation = CO for compound Phenanthrene in sample Dec2805.D; previous value =			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	12/29/2021 8:31:27 AM	Split peak for compound Anthracene in sample Dec2805.D and keep right peak, new integration is from x, y = 9.867, 92.9087593565855 to 9.916, 92.9087593565855 and new response = 16813, previous integration is from x, y = 9.780, 93 to 9.916, 93 and previous response = 38338.			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	12/29/2021 8:31:29 AM	Split qualifier 176.0 of compound Anthracene in sample Dec2805.D and keep right peak, new integration is from x, y = 9.867, 69.237035002035 to 9.916, 69.237035002035 and new response = 3073, previous integration is from x, y = 9.780, 69 to 9.916, 69 and previous response = 7091.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:31:31 AM	Set UserAnnotation = CO for compound Anthracene in sample Dec2805.D; previous value =			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 8:31:36 AM	Manually integrate qualifier 101.0 of compound Fluoranthene in sample Dec2805.D from x, y = 11.411, 109 to 11.547, 323; result = 1490			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	12/29/2021 8:31:38 AM	Snap baseline for qualifier 101.0 of compound Fluoranthene in sample Dec2805.D from x = 11.411 to x = 11.547, new integration is from x, y = 11.411, 73 to 11.547, 92 and new response = 2576; previous integration is from x, y = 11.411, 109 to 11.547, 323 and previous response = 1490.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 8:31:38 AM	Drop baseline for qualifier 101.0 of compound Fluoranthene in sample Dec2805.D to y = 73, new integration is from x, y = 11.411, 73 to 11.547, 73 and new response = 2653; previous integration is from x, y = 11.411, 73 to 11.547, 92 and previous response = 2576.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 8:32:08 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Dec2806.D, from x, y = 5.978, 344 to 6.053, 99, result = 1085; previous integration is from x, y = 5.941, 99 to 6.053, 99 and previous response = 6827.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 8:32:09 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Dec2806.D to y = 99, new integration is from x, y = 5.978, 99 to 6.053, 99 and new response = 1636; previous integration is from x, y = 5.978, 344 to 6.053, 99 and previous response = 1085.			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	12/29/2021 8:32:22 AM	Split peak for compound Phenanthrene in sample Dec2806.D and keep left peak, new integration is from x, y = 9.780, 90.1648378191857 to 9.867, 90.1648378191857 and new response = 10788, previous integration is from x, y = 9.780, 90 to 9.965, 90 and previous response = 19679.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:32:26 AM	Set UserAnnotation = CO for compound Phenanthrene in sample Dec2806.D; previous value =			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	12/29/2021 8:32:31 AM	Split peak for compound Anthracene in sample Dec2806.D and keep right peak, new integration is from x, y = 9.867, 90.1648378191857 to 9.965, 90.1648378191857 and new response = 8953, previous integration is from x, y = 9.780, 90 to 9.965, 90 and previous response = 19679.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:32:33 AM	Set UserAnnotation = CO for compound Anthracene in sample Dec2806.D; previous value =			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 8:33:05 AM	Manually integrate qualifier 129.0 of compound Naphthalene in sample Dec2807.D, from x, y = 5.978, 143 to 6.041, 129, result = 368; previous integration is from x, y = 5.946, 129 to 6.041, 129 and previous response = 502.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 8:33:07 AM	Drop baseline for qualifier 129.0 of compound Naphthalene in sample Dec2807.D to y = 129, new integration is from x, y = 5.978, 129 to 6.041, 129 and new response = 396; previous integration is from x, y = 5.978, 143 to 6.041, 129 and previous response = 368.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 8:33:10 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Dec2807.D, from x, y = 5.978, 273 to 6.053, 104, result = 457; previous integration is from x, y = 5.941, 103 to 6.053, 104 and previous response = 5869.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 8:33:11 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Dec2807.D to y = 104, new integration is from x, y = 5.978, 104 to 6.053, 104 and new response = 839; previous integration is from x, y = 5.978, 273 to 6.053, 104 and previous response = 457.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 8:33:26 AM	Manually integrate qualifier 142.0 of compound 1-Methylnaphthalene in sample Dec2807.D from x, y = 6.902, 323 to 7.015, 274; result = 971			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	12/29/2021 8:33:27 AM	Snap baseline for qualifier 142.0 of compound 1-Methylnaphthalene in sample Dec2807.D from x = 6.902 to x = 7.015, new integration is from x, y = 6.902, 170 to 7.015, 125 and new response = 1992; previous integration is from x, y = 6.902, 323 to 7.015, 274 and previous response = 971.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 8:33:28 AM	Drop baseline for qualifier 142.0 of compound 1-Methylnaphthalene in sample Dec2807.D to y = 125, new integration is from x, y = 6.902, 125 to 7.015, 125 and new response = 2144; previous integration is from x, y = 6.902, 170 to 7.015, 125 and previous response = 1992.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 8:33:31 AM	Manually integrate qualifier 115.0 of compound 1-Methylnaphthalene in sample Dec2807.D, from x, y = 6.902, 294 to 6.965, 311, result = 904; previous integration is from x, y = 6.877, 227 to 7.052, 224 and previous response = 1292.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	12/29/2021 8:33:33 AM	Snap baseline for qualifier 115.0 of compound 1-Methylnaphthalene in sample Dec2807.D from x = 6.902 to x = 6.965, new integration is from x, y = 6.902, 247 to 6.965, 240 and new response = 1125; previous integration is from x, y = 6.902, 294 to 6.965, 311 and previous response = 904.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 8:33:34 AM	Drop baseline for qualifier 115.0 of compound 1-Methylnaphthalene in sample Dec2807.D to y = 240, new integration is from x, y = 6.902, 240 to 6.965, 240 and new response = 1138; previous integration is from x, y = 6.902, 247 to 6.965, 240 and previous response = 1125.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	12/29/2021 8:33:42 AM	Manually integrate compound Acenaphthene in sample Dec2807.D, from x, y = 8.187, 1225 to 8.200, 1252, result = -849; previous integration is from x, y = 8.001, 83 to 8.150, 84 and previous response = 4063.			✓	
CmdClearManualIntegration	BL2000\jheine	12/29/2021 8:33:46 AM	Clear manual integration of target signal for compound Acenaphthene in sample Dec2807.D			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	12/29/2021 8:33:48 AM	Split peak for compound Acenaphthene in sample Dec2807.D and keep right peak, new integration is from x, y = 8.001, 82.6967195098868 to 8.150, 84.3988008776998 and new response = 4063, previous integration is from x, y = 8.001, 83 to 8.150, 84 and previous response = 4063.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	12/29/2021 8:33:55 AM	Manually integrate compound Acenaphthene in sample Dec2807.D, from x, y = 8.050, 160 to 8.150, 84, result = 2267; previous integration is from x, y = 8.001, 83 to 8.150, 84 and previous response = 4063.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 8:33:57 AM	Drop baseline for compound Acenaphthene in sample Dec2807.D to y = 84, new integration is from x, y = 8.050, 84 to 8.150, 84 and new response = 2494; previous integration is from x, y = 8.050, 160 to 8.150, 84 and previous response = 2267.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:33:59 AM	Set UserAnnotation = CO for compound Acenaphthene in sample Dec2807.D; previous value =			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 8:34:01 AM	Manually integrate qualifier 152.0 of compound Acenaphthene in sample Dec2807.D, from x, y = 8.038, 210 to 8.088, 282, result = 845; previous integration is from x, y = 7.826, 95 to 7.938, 95 and previous response = 3311.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	12/29/2021 8:34:03 AM	Snap baseline for qualifier 152.0 of compound Acenaphthene in sample Dec2807.D from x = 8.038 to x = 8.088, new integration is from x, y = 8.038, 113 to 8.088, 136 and new response = 1208; previous integration is from x, y = 8.038, 210 to 8.088, 282 and previous response = 845.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 8:34:04 AM	Drop baseline for qualifier 152.0 of compound Acenaphthene in sample Dec2807.D to y = 113, new integration is from x, y = 8.038, 113 to 8.088, 113 and new response = 1243; previous integration is from x, y = 8.038, 113 to 8.088, 136 and previous response = 1208.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 8:34:30 AM	Manually integrate qualifier 138.0 of compound Indeno(1,2,3-cd)pyrene in sample Dec2807.D, from x, y = 20.217, 192 to 20.303, 204, result = 486; previous integration is from x, y = 20.243, 237 to 20.299, 243 and previous response = 289.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 8:34:31 AM	Drop baseline for qualifier 138.0 of compound Indeno(1,2,3-cd)pyrene in sample Dec2807.D to y = 192, new integration is from x, y = 20.217, 192 to 20.303, 192 and new response = 517; previous integration is from x, y = 20.217, 192 to 20.303, 204 and previous response = 486.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 8:35:48 AM	Manually integrate qualifier 139.0 of compound Dibenzo(a,h)anthracene in sample Dec2807.D, from x, y = 20.296, 187 to 20.365, 230, result = 325; previous integration is from x, y = 20.296, 187 to 20.489, 205 and previous response = 621.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 8:35:50 AM	Drop baseline for qualifier 139.0 of compound Dibenzo(a,h)anthracene in sample Dec2807.D to y = 187, new integration is from x, y = 20.296, 187 to 20.365, 187 and new response = 415; previous integration is from x, y = 20.296, 187 to 20.365, 230 and previous response = 325.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 8:35:59 AM	Manually integrate qualifier 138.0 of compound Benzo(g,h,i)perylene in sample Dec2807.D, from x, y = 20.563, 251 to 20.649, 247, result = 552; previous integration is from x, y = 20.570, 272 to 20.628, 281 and previous response = 431.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 8:36:01 AM	Drop baseline for qualifier 138.0 of compound Benzo(g,h,i)perylene in sample Dec2807.D to y = 247, new integration is from x, y = 20.563, 247 to 20.649, 247 and new response = 562; previous integration is from x, y = 20.563, 251 to 20.649, 247 and previous response = 552.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 8:36:10 AM	Manually integrate qualifier 128.0 of compound Nitrobenzene-d5 in sample Dec2807.D, from x, y = 5.168, 202 to 5.267, 204, result = 316; previous integration is from x, y = 5.168, 202 to 5.354, 188 and previous response = 446.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 8:36:12 AM	Drop baseline for qualifier 128.0 of compound Nitrobenzene-d5 in sample Dec2807.D to y = 202, new integration is from x, y = 5.168, 202 to 5.267, 202 and new response = 322; previous integration is from x, y = 5.168, 202 to 5.267, 204 and previous response = 316.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 8:36:26 AM	Manually integrate qualifier 129.0 of compound Naphthalene in sample Dec2808.D, from x, y = 5.978, 148 to 6.028, 134, result = 206; previous integration is from x, y = 5.945, 135 to 6.028, 134 and previous response = 330.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 8:36:28 AM	Drop baseline for qualifier 129.0 of compound Naphthalene in sample Dec2808.D to y = 134, new integration is from x, y = 5.978, 134 to 6.028, 134 and new response = 228; previous integration is from x, y = 5.978, 148 to 6.028, 134 and previous response = 206.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 8:36:31 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Dec2808.D, from x, y = 5.978, 200 to 6.041, 98, result = 396; previous integration is from x, y = 5.941, 98 to 6.041, 98 and previous response = 5557.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 8:36:32 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Dec2808.D to y = 98, new integration is from x, y = 5.978, 98 to 6.041, 98 and new response = 586; previous integration is from x, y = 5.978, 200 to 6.041, 98 and previous response = 396.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 8:36:42 AM	Manually integrate qualifier 142.0 of compound 1-Methylnaphthalene in sample Dec2808.D from x, y = 6.902, 209 to 7.015, 220; result = 598			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	12/29/2021 8:36:44 AM	Snap baseline for qualifier 142.0 of compound 1-Methylnaphthalene in sample Dec2808.D from x = 6.902 to x = 7.015, new integration is from x, y = 6.902, 142 to 7.015, 109 and new response = 1198; previous integration is from x, y = 6.902, 209 to 7.015, 220 and previous response = 598.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 8:36:45 AM	Drop baseline for qualifier 142.0 of compound 1-Methylnaphthalene in sample Dec2808.D to y = 109, new integration is from x, y = 6.902, 109 to 7.015, 109 and new response = 1309; previous integration is from x, y = 6.902, 142 to 7.015, 109 and previous response = 1198.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 8:36:49 AM	Manually integrate qualifier 115.0 of compound 1-Methylnaphthalene in sample Dec2808.D, from x, y = 6.877, 227 to 6.977, 264, result = 627; previous integration is from x, y = 6.877, 227 to 7.019, 224 and previous response = 769.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 8:36:50 AM	Drop baseline for qualifier 115.0 of compound 1-Methylnaphthalene in sample Dec2808.D to y = 227, new integration is from x, y = 6.877, 227 to 6.977, 227 and new response = 738; previous integration is from x, y = 6.877, 227 to 6.977, 264 and previous response = 627.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	12/29/2021 8:37:00 AM	Manually integrate compound Acenaphthene in sample Dec2808.D, from x, y = 8.050, 163 to 8.100, 87, result = 1292; previous integration is from x, y = 8.002, 88 to 8.100, 87 and previous response = 3082.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 8:37:02 AM	Drop baseline for compound Acenaphthene in sample Dec2808.D to y = 87, new integration is from x, y = 8.050, 87 to 8.100, 87 and new response = 1406; previous integration is from x, y = 8.050, 163 to 8.100, 87 and previous response = 1292.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 8:37:05 AM	Manually integrate qualifier 152.0 of compound Acenaphthene in sample Dec2808.D, from x, y = 8.038, 160 to 8.088, 276, result = 399; previous integration is from x, y = 7.826, 95 to 7.938, 95 and previous response = 1955.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	12/29/2021 8:37:06 AM	Snap baseline for qualifier 152.0 of compound Acenaphthene in sample Dec2808.D from x = 8.038 to x = 8.088, new integration is from x, y = 8.038, 101 to 8.088, 117 and new response = 726; previous integration is from x, y = 8.038, 160 to 8.088, 276 and previous response = 399.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 8:37:07 AM	Drop baseline for qualifier 152.0 of compound Acenaphthene in sample Dec2808.D to y = 101, new integration is from x, y = 8.038, 101 to 8.088, 101 and new response = 750; previous integration is from x, y = 8.038, 101 to 8.088, 117 and previous response = 726.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:37:10 AM	Set UserAnnotation = CO for compound Acenaphthene in sample Dec2808.D; previous value =			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	12/29/2021 8:37:18 AM	Split qualifier 176.0 of compound Phenanthrene in sample Dec2808.D and keep left peak, new integration is from x, y = 9.785, 68.1670873397436 to 9.867, 68.1670873397436 and new response = 486, previous integration is from x, y = 9.785, 68 to 9.916, 68 and previous response = 813.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 8:37:28 AM	Manually integrate qualifier 176.0 of compound Anthracene in sample Dec2808.D from x, y = 9.867, 92 to 9.941, 110; result = 207			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	12/29/2021 8:37:30 AM	Snap baseline for qualifier 176.0 of compound Anthracene in sample Dec2808.D from x = 9.867 to x = 9.941, new integration is from x, y = 9.867, 73 to 9.941, 74 and new response = 330; previous integration is from x, y = 9.867, 92 to 9.941, 110 and previous response = 207.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 8:37:31 AM	Drop baseline for qualifier 176.0 of compound Anthracene in sample Dec2808.D to y = 73, new integration is from x, y = 9.867, 73 to 9.941, 73 and new response = 332; previous integration is from x, y = 9.867, 73 to 9.941, 74 and previous response = 330.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 8:37:52 AM	Manually integrate qualifier 253.0 of compound Benzo(a)pyrene in sample Dec2808.D, from x, y = 18.388, 149 to 18.475, 161, result = 276; previous integration is from x, y = 18.399, 170 to 18.463, 174 and previous response = 193.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 8:37:54 AM	Drop baseline for qualifier 253.0 of compound Benzo(a)pyrene in sample Dec2808.D to y = 149, new integration is from x, y = 18.388, 149 to 18.475, 149 and new response = 307; previous integration is from x, y = 18.388, 149 to 18.475, 161 and previous response = 276.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 8:38:03 AM	Manually integrate qualifier 138.0 of compound Indeno(1,2,3-cd)pyrene in sample Dec2808.D, from x, y = 20.229, 202 to 20.303, 216, result = 269; previous integration is from x, y = 20.240, 216 to 20.302, 234 and previous response = 188.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 8:38:04 AM	Drop baseline for qualifier 138.0 of compound Indeno(1,2,3-cd)pyrene in sample Dec2808.D to y = 202, new integration is from x, y = 20.229, 202 to 20.303, 202 and new response = 299; previous integration is from x, y = 20.229, 202 to 20.303, 216 and previous response = 269.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 8:38:12 AM	Manually integrate qualifier 139.0 of compound Dibenzo(a,h)anthracene in sample Dec2808.D, from x, y = 20.300, 196 to 20.390, 213, result = 244; previous integration is from x, y = 20.300, 196 to 20.487, 215 and previous response = 352.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 8:38:14 AM	Drop baseline for qualifier 139.0 of compound Dibenzo(a,h)anthracene in sample Dec2808.D to y = 196, new integration is from x, y = 20.300, 196 to 20.390, 196 and new response = 291; previous integration is from x, y = 20.300, 196 to 20.390, 213 and previous response = 244.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 8:38:21 AM	Manually integrate qualifier 138.0 of compound Benzo(g,h,i)perylene in sample Dec2808.D, from x, y = 20.563, 306 to 20.649, 289, result = 110; previous integration is from x, y = 20.509, 256 to 20.627, 262 and previous response = 404.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateS napBaseline	BL2000\jheine	12/29/2021 8:38:23 AM	Snap baseline for qualifier 138.0 of compound Benzo(g,h,i)perylene in sample Dec2808.D from x = 20.563 to x = 20.649, new integration is from x, y = 20.563, 299 to 20.649, 237 and new response = 262; previous integration is from x, y = 20.563, 306 to 20.649, 289 and previous response = 110.			✓	
CmdManuallyIntegrate DropBaseline	BL2000\jheine	12/29/2021 8:38:23 AM	Drop baseline for qualifier 138.0 of compound Benzo(g,h,i)perylene in sample Dec2808.D to y = 237, new integration is from x, y = 20.563, 237 to 20.649, 237 and new response = 423; previous integration is from x, y = 20.563, 299 to 20.649, 237 and previous response = 262.			✓	
CmdManuallyIntegrate QualifierPeak	BL2000\jheine	12/29/2021 8:38:47 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Dec2809.D, from x, y = 5.978, 850 to 6.107, 135, result = 3114; previous integration is from x, y = 5.928, 106 to 6.107, 135 and previous response = 12503.			✓	
CmdManuallyIntegrate DropBaseline	BL2000\jheine	12/29/2021 8:38:49 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Dec2809.D to y = 135, new integration is from x, y = 5.978, 135 to 6.107, 135 and new response = 5870; previous integration is from x, y = 5.978, 850 to 6.107, 135 and previous response = 3114.			✓	
CmdManuallyIntegrate QualifierPeak	BL2000\jheine	12/29/2021 8:39:01 AM	Manually integrate qualifier 152.0 of compound Acenaphthene in sample Dec2809.D from x, y = 8.025, 3893 to 8.100, 4999; result = -3591			✓	
CmdManuallyIntegrateS napBaseline	BL2000\jheine	12/29/2021 8:39:03 AM	Snap baseline for qualifier 152.0 of compound Acenaphthene in sample Dec2809.D from x = 8.025 to x = 8.100, new integration is from x, y = 8.025, 192 to 8.100, 405 and new response = 15013; previous integration is from x, y = 8.025, 3893 to 8.100, 4999 and previous response = -3591.			✓	
CmdManuallyIntegrate DropBaseline	BL2000\jheine	12/29/2021 8:39:04 AM	Drop baseline for qualifier 152.0 of compound Acenaphthene in sample Dec2809.D to y = 192, new integration is from x, y = 8.025, 192 to 8.100, 192 and new response = 15491; previous integration is from x, y = 8.025, 192 to 8.100, 405 and previous response = 15013.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdCalibrate	BL2000\jheine	12/29/2021 8:39:47 AM	Replace level ICV with QC sample Dec2809.D for compounds {Benzo(g,h,i)perylene, Dibenzo(a,h)anthracene, Indeno(1,2,3-cd)pyrene, Benzo(a)pyrene, Benzo(k)fluoranthene, Benzo(b)fluoranthene, Chrysene, Benzo(a)Anthracene, Terphenyl-d14, Pyrene, Fluoranthene, Anthracene, Phenanthrene, Fluorene, Acenaphthene, Acenaphthylene, 2-Fluorobiphenyl, 1-Methylnaphthalene, 2-Methylnaphthalene, Naphthalene, Nitrobenzene-d5, o-Terphenyl}; Replace level 1 with Calibration sample Dec2808.D for compounds {Benzo(g,h,i)perylene, Dibenzo(a,h)anthracene, Indeno(1,2,3-cd)pyrene, Benzo(a)pyrene, Benzo(k)fluoranthene, Benzo(b)fluoranthene, Chrysene, Benzo(a)Anthracene, Terphenyl-d14, Pyrene, Fluoranthene, Anthracene, Phenanthrene, Fluorene, Acenaphthene, Acenaphthylene, 2-Fluorobiphenyl, 1-Methylnaphthalene, 2-Methylnaphthalene, Naphthalene, Nitrobenzene-d5, o-Terphenyl}; Replace level 2 with Calibration sample Dec2807.D for compounds {Benzo(g,h,i)perylene, Dibenzo(a,h)anthracene, Indeno(1,2,3-cd)pyrene, Benzo(a)pyrene, Benzo(k)fluoranthene, Benzo(b)fluoranthene, Chrysene, Benzo(a)Anthracene, Terphenyl-d14, Pyrene, Fluoranthene, Anthracene, Phenanthrene, Fluorene, Acenaphthene, Acenaphthylene, 2-Fluorobiphenyl, 1-Methylnaphthalene, 2-Methylnaphthalene, Naphthalene, Nitrobenzene-d5, o-Terphenyl}; Replace level 3 with Calibration sample Dec2806.D for compounds {Benzo(g,h,i)perylene, Dibenzo(a,h)anthracene, Indeno(1,2,3-cd)pyrene, Benzo(a)pyrene, Benzo(k)fluoranthene, Benzo(b)fluoranthene, Chrysene, Benzo(a)Anthracene, Terphenyl-d14, Pyrene, Fluoranthene, Anthracene, Phenanthrene, Fluorene, Acenaphthene, Acenaphthylene, 2-Fluorobiphenyl, 1-Methylnaphthalene, 2-Methylnaphthalene, Naphthalene, Nitrobenzene-d5, o-Terphenyl};			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
			Nitrobenzene-d5, o-Terphenyl}; Replace level 4 with Calibration sample Dec2805.D for compounds {Benzo(g,h,i)perylene, Dibenzo(a,h)anthracene, Indeno(1,2,3-cd)pyrene, Benzo(a)pyrene, Benzo(k)fluoranthene, Benzo(b)fluoranthene, Chrysene, Benzo(a)Anthracene, Terphenyl-d14, Pyrene, Fluoranthene, Anthracene, Phenanthrene, Fluorene, Acenaphthene, Acenaphthylene, 2- Fluorobiphenyl, 1-Methylnaphthalene, 2-Methylnaphthalene, Naphthalene, Nitrobenzene-d5, o-Terphenyl}; Replace level 5 with Calibration sample Dec2804.D for compounds {Benzo(g,h,i)perylene, Dibenzo(a,h)anthracene, Indeno(1,2,3-cd)pyrene, Benzo(a)pyrene, Benzo(k)fluoranthene, Benzo(b)fluoranthene, Chrysene, Benzo(a)Anthracene, Terphenyl-d14, Pyrene, Fluoranthene, Anthracene, Phenanthrene, Fluorene, Acenaphthene, Acenaphthylene, 2- Fluorobiphenyl, 1-Methylnaphthalene, 2-Methylnaphthalene, Naphthalene, Nitrobenzene-d5, o-Terphenyl}; Replace level 6 with Calibration sample Dec2803.D for compounds {Benzo(g,h,i)perylene, Dibenzo(a,h)anthracene, Indeno(1,2,3-cd)pyrene, Benzo(a)pyrene, Benzo(k)fluoranthene, Benzo(b)fluoranthene, Chrysene, Benzo(a)Anthracene, Terphenyl-d14, Pyrene, Fluoranthene, Anthracene, Phenanthrene, Fluorene, Acenaphthene, Acenaphthylene, 2- Fluorobiphenyl, 1-Methylnaphthalene, 2-Methylnaphthalene, Naphthalene, Nitrobenzene-d5, o-Terphenyl}; Replace level 7 with Calibration sample Dec2802.D for compounds {Benzo(g,h,i)perylene, Dibenzo(a,h)anthracene, Indeno(1,2,3-cd)pyrene, Benzo(a)pyrene, Benzo(k)fluoranthene, Benzo(b)fluoranthene, Chrysene, Benzo(a)Anthracene, Terphenyl-d14, Pyrene, Fluoranthene, Anthracene, Phenanthrene, Fluorene, Acenaphthene, Acenaphthylene, 2- Fluorobiphenyl, 1-Methylnaphthalene,				

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
			2-Methylnaphthalene, Naphthalene, Nitrobenzene-d5, o-Terphenyl};				
CmdQuantitate	BL2000\jheine	12/29/2021 8:40:01 AM	Quantitate all compounds in all samples			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:40:38 AM	Set CurveFit = fitAverageOfResponseFactors for compound Nitrobenzene-d5 in all samples; previous value = fitQuadratic			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:40:42 AM	Set CurveFitOrigin = originIgnore for compound Nitrobenzene-d5 in all samples; previous value = originInclude			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:40:45 AM	Set CurveFitWeight = weightEqual for compound Nitrobenzene-d5 in all samples; previous value = weightOneOverX			✓	
CmdQuantitate	BL2000\jheine	12/29/2021 8:40:57 AM	Quantitate all compounds in all samples			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:41:05 AM	Set CurveFit = fitQuadratic for compound Nitrobenzene-d5 in all samples; previous value = fitQuadratic			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:41:10 AM	Set CurveFitOrigin = originInclude for compound Nitrobenzene-d5 in all samples; previous value = originInclude			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:41:13 AM	Set CurveFitWeight = weightOneOverX for compound Nitrobenzene-d5 in all samples; previous value = weightOneOverX			✓	
CmdQuantitate	BL2000\jheine	12/29/2021 8:41:27 AM	Quantitate all compounds in all samples			✓	
CmdManuallyIntegratePeak	BL2000\jheine	12/29/2021 8:41:46 AM	Manually integrate compound 1,4-Dichlorobenzene-d4 in sample Dec2809.D, from x, y = 4.534, 144 to 5.516, 351, result = 325055; previous integration is from x, y = 4.534, 144 to 4.646, 147 and previous response = 320765.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 8:41:48 AM	Drop baseline for compound 1,4-Dichlorobenzene-d4 in sample Dec2809.D to y = 144, new integration is from x, y = 4.534, 144 to 5.516, 144 and new response = 331151; previous integration is from x, y = 4.534, 144 to 5.516, 351 and previous response = 325055.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	12/29/2021 8:42:08 AM	Manually integrate compound Nitrobenzene-d5 in sample Dec2809.D, from x, y = 5.168, 564 to 5.305, 756, result = 16405; previous integration is from x, y = 5.168, 399 to 5.330, 428 and previous response = 18569.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateS napBaseline	BL2000\jheine	12/29/2021 8:42:11 AM	Snap baseline for compound Nitrobenzene-d5 in sample Dec2809.D, from x = 5.168 to x = 5.305, new integration is from x, y = 5.168, 404 to 5.305, 519 and new response = 18031; previous integration is from x, y = 5.168, 564 to 5.305, 756 and previous response = 16405.			✓	
CmdManuallyIntegrate DropBaseline	BL2000\jheine	12/29/2021 8:42:11 AM	Drop baseline for compound Nitrobenzene-d5 in sample Dec2809.D to y = 404, new integration is from x, y = 5.168, 404 to 5.305, 404 and new response = 18503; previous integration is from x, y = 5.168, 404 to 5.305, 519 and previous response = 18031.			✓	
CmdSetTargetCompoun dAttribute	BL2000\jheine	12/29/2021 8:42:28 AM	Set CurveFit = fitAverageOfResponseFactors for compound Naphthalene in all samples; previous value = fitQuadratic			✓	
CmdSetTargetCompoun dAttribute	BL2000\jheine	12/29/2021 8:42:32 AM	Set CurveFitOrigin = originIgnore for compound Naphthalene in all samples; previous value = originInclude			✓	
CmdSetTargetCompoun dAttribute	BL2000\jheine	12/29/2021 8:42:35 AM	Set CurveFitWeight = weightEqual for compound Naphthalene in all samples; previous value = weightOneOverX			✓	
CmdQuantitate	BL2000\jheine	12/29/2021 8:42:44 AM	Quantitate all compounds in all samples			✓	
CmdSetTargetCompoun dAttribute	BL2000\jheine	12/29/2021 8:42:57 AM	Set CurveFit = fitAverageOfResponseFactors for compound 2-Methylnaphthalene in all samples; previous value = fitQuadratic			✓	
CmdSetTargetCompoun dAttribute	BL2000\jheine	12/29/2021 8:43:01 AM	Set CurveFitOrigin = originIgnore for compound 2-Methylnaphthalene in all samples; previous value = originInclude			✓	
CmdSetTargetCompoun dAttribute	BL2000\jheine	12/29/2021 8:43:04 AM	Set CurveFitWeight = weightEqual for compound 2-Methylnaphthalene in all samples; previous value = weightOneOverX			✓	
CmdQuantitate	BL2000\jheine	12/29/2021 8:43:14 AM	Quantitate all compounds in all samples			✓	
CmdSetTargetCompoun dAttribute	BL2000\jheine	12/29/2021 8:43:29 AM	Set CurveFit = fitAverageOfResponseFactors for compound 1-Methylnaphthalene in all samples; previous value = fitQuadratic			✓	
CmdSetTargetCompoun dAttribute	BL2000\jheine	12/29/2021 8:43:31 AM	Set CurveFitOrigin = originIgnore for compound 1-Methylnaphthalene in all samples; previous value = originInclude			✓	
CmdSetTargetCompoun dAttribute	BL2000\jheine	12/29/2021 8:43:33 AM	Set CurveFitWeight = weightEqual for compound 1-Methylnaphthalene in all samples; previous value = weightOneOverX			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdQuantitate	BL2000\jheine	12/29/2021 8:43:44 AM	Quantitate all compounds in all samples			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:43:58 AM	Set CurveFit = fitAverageOfResponseFactors for compound Acenaphthylene in all samples; previous value = fitQuadratic			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:44:01 AM	Set CurveFitOrigin = originIgnore for compound Acenaphthylene in all samples; previous value = originInclude			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:44:03 AM	Set CurveFitWeight = weightEqual for compound Acenaphthylene in all samples; previous value = weightOneOverX			✓	
CmdQuantitate	BL2000\jheine	12/29/2021 8:44:14 AM	Quantitate all compounds in all samples			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:44:33 AM	Set CurveFit = fitAverageOfResponseFactors for compound Acenaphthene in all samples; previous value = fitQuadratic			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:44:37 AM	Set CurveFitOrigin = originIgnore for compound Acenaphthene in all samples; previous value = originInclude			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:44:39 AM	Set CurveFitWeight = weightEqual for compound Acenaphthene in all samples; previous value = weightOneOverXSquared			✓	
CmdQuantitate	BL2000\jheine	12/29/2021 8:44:51 AM	Quantitate all compounds in all samples			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:45:05 AM	Set CurveFit = fitAverageOfResponseFactors for compound Fluorene in all samples; previous value = fitQuadratic			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:45:09 AM	Set CurveFitOrigin = originIgnore for compound Fluorene in all samples; previous value = originInclude			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:45:12 AM	Set CurveFitWeight = weightEqual for compound Fluorene in all samples; previous value = weightOneOverX			✓	
CmdQuantitate	BL2000\jheine	12/29/2021 8:45:25 AM	Quantitate all compounds in all samples			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:45:37 AM	Set CurveFit = fitAverageOfResponseFactors for compound 2-Fluorobiphenyl in all samples; previous value = fitQuadratic			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:45:41 AM	Set CurveFitOrigin = originIgnore for compound 2-Fluorobiphenyl in all samples; previous value = originInclude			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:45:44 AM	Set CurveFitWeight = weightEqual for compound 2-Fluorobiphenyl in all samples; previous value = weightOneOverX			✓	
CmdQuantitate	BL2000\jheine	12/29/2021 8:45:53 AM	Quantitate all compounds in all samples			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:46:05 AM	Set CurveFit = fitAverageOfResponseFactors for compound Phenanthrene in all samples; previous value = fitQuadratic			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:46:07 AM	Set CurveFitOrigin = originIgnore for compound Phenanthrene in all samples; previous value = originInclude			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:46:09 AM	Set CurveFitWeight = weightEqual for compound Phenanthrene in all samples; previous value = weightOneOverX			✓	
CmdQuantitate	BL2000\jheine	12/29/2021 8:46:20 AM	Quantitate all compounds in all samples			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:46:27 AM	Set CurveFit = fitQuadratic for compound Phenanthrene in all samples; previous value = fitQuadratic			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:46:31 AM	Set CurveFitOrigin = originInclude for compound Phenanthrene in all samples; previous value = originInclude			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:46:36 AM	Set CurveFitWeight = weightOneOverX for compound Phenanthrene in all samples; previous value = weightOneOverX			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:46:40 AM	Set CurveFitWeight = weightOneOverXSquared for compound Phenanthrene in all samples; previous value = weightOneOverX			✓	
CmdQuantitate	BL2000\jheine	12/29/2021 8:46:53 AM	Quantitate all compounds in all samples			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:47:04 AM	Set CurveFit = fitQuadratic for compound Anthracene in all samples; previous value = fitAverageOfResponseFactors			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:47:07 AM	Set CurveFitOrigin = originInclude for compound Anthracene in all samples; previous value = originIgnore			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:47:10 AM	Set CurveFitWeight = weightOneOverX for compound Anthracene in all samples; previous value = weightEqual			✓	
CmdQuantitate	BL2000\jheine	12/29/2021 8:47:20 AM	Quantitate all compounds in all samples			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:47:32 AM	Set CurveFit = fitAverageOfResponseFactors for compound Fluoranthene in all samples; previous value = fitQuadratic			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:47:35 AM	Set CurveFitOrigin = originIgnore for compound Fluoranthene in all samples; previous value = originInclude			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:47:38 AM	Set CurveFitWeight = weightEqual for compound Fluoranthene in all samples; previous value = weightOneOverX			✓	
CmdQuantitate	BL2000\jheine	12/29/2021 8:47:49 AM	Quantitate all compounds in all samples			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:48:00 AM	Set CurveFit = fitQuadratic for compound o-Terphenyl in all samples; previous value = fitAverageOfResponseFactors			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:48:06 AM	Set CurveFitOrigin = originInclude for compound o-Terphenyl in all samples; previous value = originIgnore			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:48:08 AM	Set CurveFitWeight = weightOneOverX for compound o-Terphenyl in all samples; previous value = weightEqual			✓	
CmdQuantitate	BL2000\jheine	12/29/2021 8:48:18 AM	Quantitate all compounds in all samples			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:48:24 AM	Set CurveFit = fitAverageOfResponseFactors for compound o-Terphenyl in all samples; previous value = fitAverageOfResponseFactors			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:48:28 AM	Set CurveFitOrigin = originIgnore for compound o-Terphenyl in all samples; previous value = originIgnore			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:48:31 AM	Set CurveFitWeight = weightEqual for compound o-Terphenyl in all samples; previous value = weightEqual			✓	
CmdQuantitate	BL2000\jheine	12/29/2021 8:48:42 AM	Quantitate all compounds in all samples			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:49:12 AM	Set CurveFit = fitAverageOfResponseFactors for compound Benzo(a)Anthracene in all samples; previous value = fitQuadratic			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:49:16 AM	Set CurveFit = fitQuadratic for compound Benzo(a)Anthracene in all samples; previous value = fitQuadratic			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:49:20 AM	Set CurveFitWeight = weightOneOverX for compound Benzo(a)Anthracene in all samples; previous value = weightOneOverXSquared			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdQuantitate	BL2000\jheine	12/29/2021 8:49:32 AM	Quantitate all compounds in all samples			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:49:38 AM	Set CurveFitWeight = weightOneOverXSquared for compound Benzo(a)Anthracene in all samples; previous value = weightOneOverXSquared			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:50:59 AM	Set CurveFit = fitQuadratic for compound Chrysene in all samples; previous value = fitAverageOfResponseFactors			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:51:04 AM	Set CurveFitOrigin = originInclude for compound Chrysene in all samples; previous value = originIgnore			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:51:06 AM	Set CurveFitWeight = weightOneOverXSquared for compound Chrysene in all samples; previous value = weightEqual			✓	
CmdQuantitate	BL2000\jheine	12/29/2021 8:51:18 AM	Quantitate all compounds in all samples			✓	
CmdManuallyIntegratePeak	BL2000\jheine	12/29/2021 8:51:36 AM	Manually integrate compound Chrysene-d12 in sample Dec2809.D, from x, y = 14.702, 75 to 15.598, 2323, result = 542252; previous integration is from x, y = 14.702, 75 to 14.926, 79 and previous response = 586299.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 8:51:38 AM	Drop baseline for compound Chrysene-d12 in sample Dec2809.D to y = 75, new integration is from x, y = 14.702, 75 to 15.598, 75 and new response = 602674; previous integration is from x, y = 14.702, 75 to 15.598, 2323 and previous response = 542252.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:52:17 AM	Set CurveFit = fitAverageOfResponseFactors for compound Indeno(1,2,3-cd)pyrene in all samples; previous value = fitQuadratic			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:52:21 AM	Set CurveFitWeight = weightEqual for compound Indeno(1,2,3-cd)pyrene in all samples; previous value = weightOneOverX			✓	
CmdQuantitate	BL2000\jheine	12/29/2021 8:52:32 AM	Quantitate all compounds in all samples			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:52:47 AM	Set CurveFit = fitAverageOfResponseFactors for compound Dibenzo(a,h)anthracene in all samples; previous value = fitQuadratic			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:52:51 AM	Set CurveFitWeight = weightEqual for compound Dibenzo(a,h)anthracene in all samples; previous value = weightOneOverX			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdQuantitate	BL2000\jheine	12/29/2021 8:53:04 AM	Quantitate all compounds in all samples			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:54:00 AM	Set CurveFitWeight = weightOneOverXSquared for compound Nitrobenzene-d5 in all samples; previous value = weightOneOverX			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:54:06 AM	Set CurveFitWeight = weightOneOverX for compound Nitrobenzene-d5 in all samples; previous value = weightOneOverX			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:54:10 AM	Set CurveFitWeight = weightOneOverXSquared for compound Nitrobenzene-d5 in all samples; previous value = weightOneOverX			✓	
CmdQuantitate	BL2000\jheine	12/29/2021 8:54:26 AM	Quantitate all compounds in all samples			✓	
CmdClearManualIntegration	BL2000\jheine	12/29/2021 8:55:22 AM	Clear manual integration of target signal for compound Nitrobenzene-d5 in sample Dec2809.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	12/29/2021 8:55:44 AM	Manually integrate compound Nitrobenzene-d5 in sample Dec2804.D, from x, y = 5.168, 412 to 5.367, 408, result = 14202; previous integration is from x, y = 5.150, 377 to 5.280, 378 and previous response = 14151.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	12/29/2021 8:55:47 AM	Snap baseline for compound Nitrobenzene-d5 in sample Dec2804.D, from x = 5.168 to x = 5.367, new integration is from x, y = 5.168, 390 to 5.367, 422 and new response = 14253; previous integration is from x, y = 5.168, 412 to 5.367, 408 and previous response = 14202.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 8:55:48 AM	Drop baseline for compound Nitrobenzene-d5 in sample Dec2804.D to y = 390, new integration is from x, y = 5.168, 390 to 5.367, 390 and new response = 14443; previous integration is from x, y = 5.168, 390 to 5.367, 422 and previous response = 14253.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:55:53 AM	Set UserAnnotation = BA for compound Nitrobenzene-d5 in sample Dec2804.D; previous value =			✓	
CmdManuallyIntegratePeak	BL2000\jheine	12/29/2021 8:56:12 AM	Manually integrate compound Nitrobenzene-d5 in sample Dec2803.D, from x, y = 5.168, 427 to 5.429, 648, result = 40782; previous integration is from x, y = 5.168, 427 to 5.342, 463 and previous response = 41890.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 8:56:15 AM	Drop baseline for compound Nitrobenzene-d5 in sample Dec2803.D to y = 427, new integration is from x, y = 5.168, 427 to 5.429, 427 and new response = 42512; previous integration is from x, y = 5.168, 427 to 5.429, 648 and previous response = 40782.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:56:21 AM	Set UserAnnotation = BA for compound Nitrobenzene-d5 in sample Dec2803.D; previous value =			✓	
CmdManuallyIntegratePeak	BL2000\jheine	12/29/2021 8:56:31 AM	Manually integrate compound Nitrobenzene-d5 in sample Dec2802.D, from x, y = 5.156, 789 to 5.441, 1032, result = 87529; previous integration is from x, y = 5.131, 587 to 5.267, 629 and previous response = 91135.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	12/29/2021 8:56:34 AM	Snap baseline for compound Nitrobenzene-d5 in sample Dec2802.D, from x = 5.156 to x = 5.441, new integration is from x, y = 5.156, 789 to 5.441, 646 and new response = 90838; previous integration is from x, y = 5.156, 789 to 5.441, 1032 and previous response = 87529.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 8:56:35 AM	Drop baseline for compound Nitrobenzene-d5 in sample Dec2802.D to y = 646, new integration is from x, y = 5.156, 646 to 5.441, 646 and new response = 92065; previous integration is from x, y = 5.156, 789 to 5.441, 646 and previous response = 90838.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:56:41 AM	Set UserAnnotation = BA for compound Nitrobenzene-d5 in sample Dec2802.D; previous value =			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdCalibrate	BL2000\jheine	12/29/2021 8:56:55 AM	Replace level ICV with QC sample Dec2809.D for compounds {Benzo(g,h,i)perylene, Dibenzo(a,h)anthracene, Indeno(1,2,3-cd)pyrene, Benzo(a)pyrene, Benzo(k)fluoranthene, Benzo(b)fluoranthene, Chrysene, Benzo(a)Anthracene, Terphenyl-d14, Pyrene, Fluoranthene, o-Terphenyl, Anthracene, Phenanthrene, Fluorene, Acenaphthene, Acenaphthylene, 2-Fluorobiphenyl, 1-Methylnaphthalene, 2-Methylnaphthalene, Naphthalene, Nitrobenzene-d5}; Replace level 1 with Calibration sample Dec2808.D for compounds {Benzo(g,h,i)perylene, Dibenzo(a,h)anthracene, Indeno(1,2,3-cd)pyrene, Benzo(a)pyrene, Benzo(k)fluoranthene, Benzo(b)fluoranthene, Chrysene, Benzo(a)Anthracene, Terphenyl-d14, Pyrene, Fluoranthene, o-Terphenyl, Anthracene, Phenanthrene, Fluorene, Acenaphthene, Acenaphthylene, 2-Fluorobiphenyl, 1-Methylnaphthalene, 2-Methylnaphthalene, Naphthalene, Nitrobenzene-d5}; Replace level 2 with Calibration sample Dec2807.D for compounds {Benzo(g,h,i)perylene, Dibenzo(a,h)anthracene, Indeno(1,2,3-cd)pyrene, Benzo(a)pyrene, Benzo(k)fluoranthene, Benzo(b)fluoranthene, Chrysene, Benzo(a)Anthracene, Terphenyl-d14, Pyrene, Fluoranthene, o-Terphenyl, Anthracene, Phenanthrene, Fluorene, Acenaphthene, Acenaphthylene, 2-Fluorobiphenyl, 1-Methylnaphthalene, 2-Methylnaphthalene, Naphthalene, Nitrobenzene-d5}; Replace level 3 with Calibration sample Dec2806.D for compounds {Benzo(g,h,i)perylene, Dibenzo(a,h)anthracene, Indeno(1,2,3-cd)pyrene, Benzo(a)pyrene, Benzo(k)fluoranthene, Benzo(b)fluoranthene, Chrysene, Benzo(a)Anthracene, Terphenyl-d14, Pyrene, Fluoranthene, o-Terphenyl, Anthracene, Phenanthrene, Fluorene, Acenaphthene, Acenaphthylene, 2-Fluorobiphenyl, 1-Methylnaphthalene, 2-Methylnaphthalene, Naphthalene, Nitrobenzene-d5}; Replace level 4 with Calibration sample Dec2805.D for compounds {Benzo(g,h,i)perylene,			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
			Dibenzo(a,h)anthracene, Indeno(1,2,3-cd)pyrene, Benzo(a)pyrene, Benzo(k)fluoranthene, Benzo(b)fluoranthene, Chrysene, Benzo(a)Anthracene, Terphenyl-d14, Pyrene, Fluoranthene, o-Terphenyl, Anthracene, Phenanthrene, Fluorene, Acenaphthene, Acenaphthylene, 2- Fluorobiphenyl, 1-Methylnaphthalene, 2-Methylnaphthalene, Naphthalene, Nitrobenzene-d5}; Replace level 5 with Calibration sample Dec2804.D for compounds {Benzo(g,h,i)perylene, Dibenzo(a,h)anthracene, Indeno(1,2,3-cd)pyrene, Benzo(a)pyrene, Benzo(k)fluoranthene, Benzo(b)fluoranthene, Chrysene, Benzo(a)Anthracene, Terphenyl-d14, Pyrene, Fluoranthene, o-Terphenyl, Anthracene, Phenanthrene, Fluorene, Acenaphthene, Acenaphthylene, 2- Fluorobiphenyl, 1-Methylnaphthalene, 2-Methylnaphthalene, Naphthalene, Nitrobenzene-d5}; Replace level 6 with Calibration sample Dec2803.D for compounds {Benzo(g,h,i)perylene, Dibenzo(a,h)anthracene, Indeno(1,2,3-cd)pyrene, Benzo(a)pyrene, Benzo(k)fluoranthene, Benzo(b)fluoranthene, Chrysene, Benzo(a)Anthracene, Terphenyl-d14, Pyrene, Fluoranthene, o-Terphenyl, Anthracene, Phenanthrene, Fluorene, Acenaphthene, Acenaphthylene, 2- Fluorobiphenyl, 1-Methylnaphthalene, 2-Methylnaphthalene, Naphthalene, Nitrobenzene-d5}; Replace level 7 with Calibration sample Dec2802.D for compounds {Benzo(g,h,i)perylene, Dibenzo(a,h)anthracene, Indeno(1,2,3-cd)pyrene, Benzo(a)pyrene, Benzo(k)fluoranthene, Benzo(b)fluoranthene, Chrysene, Benzo(a)Anthracene, Terphenyl-d14, Pyrene, Fluoranthene, o-Terphenyl, Anthracene, Phenanthrene, Fluorene, Acenaphthene, Acenaphthylene, 2- Fluorobiphenyl, 1-Methylnaphthalene, 2-Methylnaphthalene, Naphthalene, Nitrobenzene-d5};				
CmdQuantitate	BL2000\jheine	12/29/2021 8:57:14 AM	Quantitate all compounds in all samples			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 8:57:24 AM	Set CurveFitWeight = weightOneOverX for compound Nitrobenzene-d5 in all samples; previous value = weightOneOverX			✓	
CmdQuantitate	BL2000\jheine	12/29/2021 8:57:38 AM	Quantitate all compounds in all samples			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 8:58:53 AM	Manually integrate qualifier 128.0 of compound Nitrobenzene-d5 in sample Dec2802.D, from x, y = 5.168, 342 to 5.392, 535, result = 22702; previous integration is from x, y = 5.168, 342 to 5.280, 344 and previous response = 19089.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 8:58:55 AM	Drop baseline for qualifier 128.0 of compound Nitrobenzene-d5 in sample Dec2802.D to y = 342, new integration is from x, y = 5.168, 342 to 5.392, 342 and new response = 23994; previous integration is from x, y = 5.168, 342 to 5.392, 535 and previous response = 22702.			✓	
CmdStartMethodEditing	BL2000\jheine	12/29/2021 9:03:06 AM	Start method editing			✓	
CmdImportMethodFromSample	BL2000\jheine	12/29/2021 9:03:06 AM	Import method from sample Dec2810.D			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:24 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:25 AM	Set PeakFilterThresholdValue = 1037.63454930473 for compound Naphthalene; previous value = 1220.58893414677			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:25 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:25 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:25 AM	Set PeakFilterThresholdValue = 112.174329251956 for qualifier 129.0 of compound Naphthalene; previous value = 137.937962245688			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:25 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:26 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:26 AM	Set PeakFilterThresholdValue = 161.337722202857 for qualifier 102.0 of compound Naphthalene; previous value = 153.470798897376			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:26 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:26 AM	No parameter change for PeakFilterThreshold			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:26 AM	Set PeakFilterThresholdValue = 588.19625396825 for compound 2-Methylnaphthalene; previous value = 797.907698888901			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:26 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:26 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:27 AM	Set PeakFilterThresholdValue = 867.611723242636 for qualifier 142.0 of compound 2-Methylnaphthalene; previous value = 1044.91457486028			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:27 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:27 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:27 AM	Set PeakFilterThresholdValue = 308.814817007921 for qualifier 115.0 of compound 2-Methylnaphthalene; previous value = 434.34685767974			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:27 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:28 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:28 AM	Set PeakFilterThresholdValue = 595.299928571425 for compound 1-Methylnaphthalene; previous value = 769.836750000014			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:28 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:28 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:28 AM	Set PeakFilterThresholdValue = 662.394921309491 for qualifier 142.0 of compound 1-Methylnaphthalene; previous value = 875.458518972315			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:28 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:29 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:29 AM	Set PeakFilterThresholdValue = 377.588666044884 for qualifier 115.0 of compound 1-Methylnaphthalene; previous value = 463.799511684384			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:29 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:29 AM	No parameter change for PeakFilterThreshold			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:29 AM	Set PeakFilterThresholdValue = 977.574997222228 for compound Acenaphthylene; previous value = 1186.19511893271			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:30 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:30 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:30 AM	Set PeakFilterThresholdValue = 142.297492641816 for qualifier 153.0 of compound Acenaphthylene; previous value = 173.965894403528			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:30 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:30 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:31 AM	Set PeakFilterThresholdValue = 702.823942203903 for compound Acenaphthene; previous value = 900.573443981482			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:31 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:31 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:31 AM	Set PeakFilterThresholdValue = 385.842848130719 for qualifier 152.0 of compound Acenaphthene; previous value = 515.109769583626			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:31 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:32 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:32 AM	Set PeakFilterThresholdValue = 806.667572980904 for qualifier 153.0 of compound Acenaphthene; previous value = 1028.47322372877			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:32 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:32 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:32 AM	Set PeakFilterThresholdValue = 756.80948412701 for compound Fluorene; previous value = 1123.40680750915			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:32 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:33 AM	No parameter change for PeakFilterThreshold			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:33 AM	Set PeakFilterThresholdValue = 729.532248155729 for qualifier 165.0 of compound Fluorene; previous value = 1044.45965513908			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:33 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:33 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:34 AM	Set PeakFilterThresholdValue = 85.20871582856 for qualifier 167.0 of compound Fluorene; previous value = 145.28247658999			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:34 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:34 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:34 AM	Set PeakFilterThresholdValue = 1378.20817410716 for compound Phenanthrene; previous value = 1819.3952628983			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:34 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:34 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:35 AM	Set PeakFilterThresholdValue = 213.984541449823 for qualifier 176.0 of compound Phenanthrene; previous value = 344.606663665418			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:35 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:35 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:35 AM	Set PeakFilterThresholdValue = 1070.77109548611 for compound Anthracene; previous value = 1240.64153798309			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:35 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:36 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:36 AM	Set PeakFilterThresholdValue = 178.157498643721 for qualifier 176.0 of compound Anthracene; previous value = 222.565166759391			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:36 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:36 AM	No parameter change for PeakFilterThreshold			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:36 AM	Set PeakFilterThresholdValue = 1280.26819717778 for compound Fluoranthene; previous value = 1666.69898064172			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:37 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:37 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:37 AM	Set PeakFilterThresholdValue = 146.018350606525 for qualifier 101.0 of compound Fluoranthene; previous value = 189.615753707063			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:37 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:37 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:37 AM	Set PeakFilterThresholdValue = 1463.19161579774 for compound Pyrene; previous value = 1766.15181188539			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:38 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:38 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:38 AM	Set PeakFilterThresholdValue = 203.253032152133 for qualifier 101.0 of compound Pyrene; previous value = 234.139431933039			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:38 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:38 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:39 AM	Set PeakFilterThresholdValue = 1853.37234592252 for compound Benzo(a)Anthracene; previous value = 2187.14348133629			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:39 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:39 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:39 AM	Set PeakFilterThresholdValue = 436.107213370423 for qualifier 229.0 of compound Benzo(a)Anthracene; previous value = 588.061329030776			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:39 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:39 AM	No parameter change for PeakFilterThreshold			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:40 AM	Set PeakFilterThresholdValue = 517.609002259047 for qualifier 226.0 of compound Benzo(a)Anthracene; previous value = 601.954035400672			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:40 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:40 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:40 AM	Set PeakFilterThresholdValue = 1409.75245176248 for compound Chrysene; previous value = 1499.07610576541			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:40 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:41 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:41 AM	Set PeakFilterThresholdValue = 446.502448884273 for qualifier 226.0 of compound Chrysene; previous value = 463.739721893155			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:41 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:41 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:41 AM	Set PeakFilterThresholdValue = 313.124961416453 for qualifier 229.0 of compound Chrysene; previous value = 327.500077290095			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:42 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:42 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:42 AM	Set PeakFilterThresholdValue = 696.285772650434 for compound Benzo(b)fluoranthene; previous value = 738.398784523359			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:42 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:42 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:43 AM	Set PeakFilterThresholdValue = 157.268065765652 for qualifier 253.0 of compound Benzo(b)fluoranthene; previous value = 177.774571398214			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:43 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:43 AM	No parameter change for PeakFilterThreshold			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:43 AM	Set PeakFilterThresholdValue = 1003.41328761145 for compound Benzo(k)fluoranthene; previous value = 787.98602124904			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:43 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:43 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:44 AM	Set PeakFilterThresholdValue = 231.172355781881 for qualifier 253.0 of compound Benzo(k)fluoranthene; previous value = 194.993833639358			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:44 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:44 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:44 AM	Set PeakFilterThresholdValue = 623.737750000004 for compound Benzo(a)pyrene; previous value = 552.668149999993			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:44 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:45 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:45 AM	Set PeakFilterThresholdValue = 147.866406529718 for qualifier 253.0 of compound Benzo(a)pyrene; previous value = 138.210110576407			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:45 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:45 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:45 AM	Set PeakFilterThresholdValue = 513.001406921189 for compound Indeno(1,2,3-cd)pyrene; previous value = 420.343134349856			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:45 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:46 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:46 AM	Set PeakFilterThresholdValue = 129.069984146015 for qualifier 138.0 of compound Indeno(1,2,3-cd)pyrene; previous value = 112.040226469621			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:46 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:46 AM	No parameter change for PeakFilterThreshold			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:46 AM	Set PeakFilterThresholdValue = 575.583630389075 for compound Dibenzo(a,h)anthracene; previous value = 503.112889084119			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:46 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:47 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:47 AM	Set PeakFilterThresholdValue = 148.80303070392 for qualifier 279.0 of compound Dibenzo(a,h)anthracene; previous value = 146.512609135596			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:47 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:47 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:47 AM	Set PeakFilterThresholdValue = 105.230153069532 for qualifier 139.0 of compound Dibenzo(a,h)anthracene; previous value = 103.54906734961			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:48 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:48 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:48 AM	Set PeakFilterThresholdValue = 850.864177295763 for compound Benzo(g,h,i)perylene; previous value = 813.179317348847			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:48 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:48 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:48 AM	Set PeakFilterThresholdValue = 169.839410707477 for qualifier 138.0 of compound Benzo(g,h,i)perylene; previous value = 162.158508080862			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:49 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:49 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:49 AM	Set PeakFilterThresholdValue = 208.343339694147 for qualifier 277.0 of compound Benzo(g,h,i)perylene; previous value = 208.08866254338			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:49 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:49 AM	No parameter change for PeakFilterThreshold			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:50 AM	Set PeakFilterThresholdValue = 257.376672942736 for compound Nitrobenzene-d5; previous value = 203.39258710255			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:50 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:50 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:50 AM	Set PeakFilterThresholdValue = 79.5320739966782 for qualifier 54.0 of compound Nitrobenzene-d5; previous value = 76.3146422156176			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:50 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:51 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:51 AM	Set PeakFilterThresholdValue = 78.2812723412894 for qualifier 128.0 of compound Nitrobenzene-d5; previous value = 62.3069909380699			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:51 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:51 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:52 AM	Set PeakFilterThresholdValue = 927.30465 for compound 2-Fluorobiphenyl; previous value = 1189.77099271562			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:52 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:52 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:52 AM	Set PeakFilterThresholdValue = 349.376072801849 for qualifier 171.0 of compound 2-Fluorobiphenyl; previous value = 429.974183834712			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:52 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:53 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:53 AM	Set PeakFilterThresholdValue = 520.464385855652 for compound Terphenyl-d14; previous value = 696.705419971298			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:53 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:53 AM	No parameter change for PeakFilterThreshold			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:53 AM	Set PeakFilterThresholdValue = 71.4811505716088 for qualifier 122.0 of compound Terphenyl-d14; previous value = 97.7789219634003			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:54 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:54 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:54 AM	Set PeakFilterThresholdValue = 708.889818118197 for compound o-Terphenyl; previous value = 1011.90080568781			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:03:54 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:54 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:55 AM	Set PeakFilterThresholdValue = 473.375347897728 for qualifier 229.0 of compound o-Terphenyl; previous value = 663.460556201189			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:55 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:55 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:55 AM	Set PeakFilterThresholdValue = 306.221532169349 for qualifier 215.0 of compound o-Terphenyl; previous value = 401.397899497459			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	12/29/2021 9:03:55 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdApplyMethodToAllSamples	BL2000\jheine	12/29/2021 9:04:21 AM	Apply method to all samples			✓	
CmdMethodClear	BL2000\jheine	12/29/2021 9:04:21 AM	Clear method			✓	
CmdEndMethodEditing	BL2000\jheine	12/29/2021 9:04:22 AM	End method editing			✓	
CmdQuantitate	BL2000\jheine	12/29/2021 9:04:33 AM	Quantitate all compounds in all samples			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:04:54 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Dec2810.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	12/29/2021 9:05:01 AM	Manually integrate compound Acenaphthene in sample Dec2810.D, from x, y = 8.050, 355 to 8.113, 78, result = -376; previous integration is from x, y = 8.001, 78 to 8.113, 78 and previous response = 2114.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 9:05:02 AM	Drop baseline for compound Acenaphthene in sample Dec2810.D to y = 78, new integration is from x, y = 8.050, 78 to 8.113, 78 and new response = 142; previous integration is from x, y = 8.050, 355 to 8.113, 78 and previous response = -376.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:05:04 AM	Zero out primary peak of compound Acenaphthene in sample Dec2810.D			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:05:06 AM	Zero out primary peak of compound Chrysene in sample Dec2810.D			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:05:08 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Dec2810.D			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:05:24 AM	Zero out primary peak of compound Fluorene in sample Dec2811.D			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:05:27 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Dec2811.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	12/29/2021 9:05:33 AM	Manually integrate compound Acenaphthene in sample Dec2811.D, from x, y = 8.050, 380 to 8.088, 102, result = -200; previous integration is from x, y = 8.001, 105 to 8.088, 102 and previous response = 2355.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 9:05:34 AM	Drop baseline for compound Acenaphthene in sample Dec2811.D to y = 102, new integration is from x, y = 8.050, 102 to 8.088, 102 and new response = 112; previous integration is from x, y = 8.050, 380 to 8.088, 102 and previous response = -200.			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:05:37 AM	Zero out primary peak of compound Acenaphthene in sample Dec2811.D			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:05:40 AM	Zero out primary peak of compound Chrysene in sample Dec2811.D			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:05:41 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Dec2811.D			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:06:01 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Dec2812.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	12/29/2021 9:06:06 AM	Manually integrate compound Benzo(a)pyrene in sample Dec2812.D, from x, y = 18.388, 173 to 18.475, 340, result = -597; previous integration is from x, y = 18.524, 0 to 18.524, 0 and previous response = 0.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	12/29/2021 9:06:07 AM	Snap baseline for compound Benzo(a)pyrene in sample Dec2812.D, from x = 18.388 to x = 18.475, new integration is from x, y = 18.388, 94 to 18.475, 103 and new response = 223; previous integration is from x, y = 18.388, 173 to 18.475, 340 and previous response = -597.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 9:06:08 AM	Drop baseline for compound Benzo(a)pyrene in sample Dec2812.D to y = 94, new integration is from x, y = 18.388, 94 to 18.475, 94 and new response = 247; previous integration is from x, y = 18.388, 94 to 18.475, 103 and previous response = 223.			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:06:10 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Dec2812.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	12/29/2021 9:06:17 AM	Manually integrate compound Acenaphthene in sample Dec2812.D, from x, y = 8.050, 510 to 8.100, 78, result = -332; previous integration is from x, y = 8.001, 78 to 8.100, 78 and previous response = 2524.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 9:06:18 AM	Drop baseline for compound Acenaphthene in sample Dec2812.D to y = 78, new integration is from x, y = 8.050, 78 to 8.100, 78 and new response = 314; previous integration is from x, y = 8.050, 510 to 8.100, 78 and previous response = -332.			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:06:20 AM	Zero out primary peak of compound Acenaphthene in sample Dec2812.D			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:06:22 AM	Zero out primary peak of compound Chrysene in sample Dec2812.D			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:06:24 AM	Zero out primary peak of compound Anthracene in sample Dec2812.D			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:06:26 AM	Zero out primary peak of compound Phenanthrene in sample Dec2812.D			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:06:27 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Dec2812.D			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 9:06:59 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Dec2813.D, from x, y = 5.978, 778 to 6.116, 117, result = 4611; previous integration is from x, y = 5.941, 117 to 6.116, 117 and previous response = 14753.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 9:07:00 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Dec2813.D to y = 117, new integration is from x, y = 5.978, 117 to 6.116, 117 and new response = 7332; previous integration is from x, y = 5.978, 778 to 6.116, 117 and previous response = 4611.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateSplit	BL2000\jheine	12/29/2021 9:07:36 AM	Split peak for compound Acenaphthene in sample Dec2814.D and keep right peak, new integration is from x, y = 8.100, 78.4217495467496 to 8.150, 78.4217495467496 and new response = 133, previous integration is from x, y = 8.000, 78 to 8.150, 78 and previous response = 4379.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	12/29/2021 9:07:43 AM	Manually integrate compound Acenaphthene in sample Dec2814.D, from x, y = 8.038, 425 to 8.150, 279, result = 716; previous integration is from x, y = 8.100, 78 to 8.150, 78 and previous response = 133.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	12/29/2021 9:07:45 AM	Snap baseline for compound Acenaphthene in sample Dec2814.D, from x = 8.038 to x = 8.150, new integration is from x, y = 8.038, 214 to 8.150, 107 and new response = 2003; previous integration is from x, y = 8.038, 425 to 8.150, 279 and previous response = 716.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 9:07:46 AM	Drop baseline for compound Acenaphthene in sample Dec2814.D to y = 107, new integration is from x, y = 8.038, 107 to 8.150, 107 and new response = 2363; previous integration is from x, y = 8.038, 214 to 8.150, 107 and previous response = 2003.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:07:47 AM	Set UserAnnotation = CO for compound Acenaphthene in sample Dec2814.D; previous value =			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 9:07:51 AM	Manually integrate qualifier 152.0 of compound Acenaphthene in sample Dec2814.D, from x, y = 8.038, 293 to 8.088, 415, result = 413; previous integration is from x, y = 7.819, 93 to 7.938, 93 and previous response = 3263.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	12/29/2021 9:07:52 AM	Snap baseline for qualifier 152.0 of compound Acenaphthene in sample Dec2814.D from x = 8.038 to x = 8.088, new integration is from x, y = 8.038, 105 to 8.088, 127 and new response = 1125; previous integration is from x, y = 8.038, 293 to 8.088, 415 and previous response = 413.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 9:07:53 AM	Drop baseline for qualifier 152.0 of compound Acenaphthene in sample Dec2814.D to y = 105, new integration is from x, y = 8.038, 105 to 8.088, 105 and new response = 1158; previous integration is from x, y = 8.038, 105 to 8.088, 127 and previous response = 1125.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 9:08:12 AM	Manually integrate qualifier 129.0 of compound Naphthalene in sample Dec2814.D, from x, y = 5.978, 237 to 6.028, 118, result = 98; previous integration is from x, y = 5.930, 115 to 6.063, 115 and previous response = 447.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 9:08:13 AM	Drop baseline for qualifier 129.0 of compound Naphthalene in sample Dec2814.D to y = 118, new integration is from x, y = 5.978, 118 to 6.028, 118 and new response = 277; previous integration is from x, y = 5.978, 237 to 6.028, 118 and previous response = 98.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 9:08:19 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Dec2814.D, from x, y = 5.978, 284 to 6.053, 90, result = 256; previous integration is from x, y = 5.941, 90 to 6.053, 90 and previous response = 6152.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 9:08:21 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Dec2814.D to y = 90, new integration is from x, y = 5.978, 90 to 6.053, 90 and new response = 693; previous integration is from x, y = 5.978, 284 to 6.053, 90 and previous response = 256.			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	12/29/2021 9:08:27 AM	Split peak for compound 2-Methylnaphthalene in sample Dec2814.D and keep left peak, new integration is from x, y = 6.783, 103.66369047619 to 6.890, 103.66369047619 and new response = 1724, previous integration is from x, y = 6.783, 104 to 7.065, 104 and previous response = 3591.			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	12/29/2021 9:08:34 AM	Split peak for compound 1-Methylnaphthalene in sample Dec2814.D and keep right peak, new integration is from x, y = 6.890, 103.66369047619 to 7.065, 103.66369047619 and new response = 1867, previous integration is from x, y = 6.783, 104 to 7.065, 104 and previous response = 3591.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 9:10:00 AM	Manually integrate qualifier 152.0 of compound Acenaphthene in sample Dec2815.D from x, y = 8.025, 5265 to 8.113, 7116; result = -9709			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateS napBaseline	BL2000\jheine	12/29/2021 9:10:01 AM	Snap baseline for qualifier 152.0 of compound Acenaphthene in sample Dec2815.D from x = 8.025 to x = 8.113, new integration is from x, y = 8.025, 213 to 8.113, 456 and new response = 20941; previous integration is from x, y = 8.025, 5265 to 8.113, 7116 and previous response = -9709.			✓	
CmdManuallyIntegrate DropBaseline	BL2000\jheine	12/29/2021 9:10:02 AM	Drop baseline for qualifier 152.0 of compound Acenaphthene in sample Dec2815.D to y = 213, new integration is from x, y = 8.025, 213 to 8.113, 213 and new response = 21577; previous integration is from x, y = 8.025, 213 to 8.113, 456 and previous response = 20941.			✓	
CmdManuallyIntegrate QualifierPeak	BL2000\jheine	12/29/2021 9:10:22 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Dec2815.D, from x, y = 5.978, 1310 to 6.115, 102, result = 1236; previous integration is from x, y = 5.928, 102 to 6.115, 102 and previous response = 14374.			✓	
CmdManuallyIntegrate DropBaseline	BL2000\jheine	12/29/2021 9:10:23 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Dec2815.D to y = 102, new integration is from x, y = 5.978, 102 to 6.115, 102 and new response = 6215; previous integration is from x, y = 5.978, 1310 to 6.115, 102 and previous response = 1236.			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:11:05 AM	Zero out primary peak of compound Fluorene in sample Dec2816.D			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:11:08 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Dec2816.D			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:11:12 AM	Zero out primary peak of compound Acenaphthene in sample Dec2816.D			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:11:15 AM	Zero out primary peak of compound Chrysene in sample Dec2816.D			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:11:16 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Dec2816.D			✓	
CmdManuallyIntegrateP eak	BL2000\jheine	12/29/2021 9:11:36 AM	Manually integrate compound Benzo(a)pyrene in sample Dec2817.D, from x, y = 18.388, 163 to 18.450, 227, result = -201; previous integration is from x, y = 18.487, 99 to 18.573, 103 and previous response = 2575.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	12/29/2021 9:11:38 AM	Snap baseline for compound Benzo(a)pyrene in sample Dec2817.D, from x = 18.388 to x = 18.450, new integration is from x, y = 18.388, 91 to 18.450, 106 and new response = 157; previous integration is from x, y = 18.388, 163 to 18.450, 227 and previous response = -201.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 9:11:38 AM	Drop baseline for compound Benzo(a)pyrene in sample Dec2817.D to y = 91, new integration is from x, y = 18.388, 91 to 18.450, 91 and new response = 185; previous integration is from x, y = 18.388, 91 to 18.450, 106 and previous response = 157.			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:11:41 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Dec2817.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	12/29/2021 9:11:55 AM	Manually integrate compound Acenaphthene in sample Dec2817.D, from x, y = 8.050, 445 to 8.113, 77, result = -363; previous integration is from x, y = 7.996, 77 to 8.113, 77 and previous response = 2611.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 9:11:56 AM	Drop baseline for compound Acenaphthene in sample Dec2817.D to y = 77, new integration is from x, y = 8.050, 77 to 8.113, 77 and new response = 324; previous integration is from x, y = 8.050, 445 to 8.113, 77 and previous response = -363.			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:11:58 AM	Zero out primary peak of compound Acenaphthene in sample Dec2817.D			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:12:01 AM	Zero out primary peak of compound Chrysene in sample Dec2817.D			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:12:02 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Dec2817.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	12/29/2021 9:12:22 AM	Manually integrate compound Naphthalene in sample Dec2818.D, from x, y = 5.966, 176 to 6.003, 5750, result = 114805; previous integration is from x, y = 5.966, 176 to 6.066, 176 and previous response = 138394.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 9:12:24 AM	Drop baseline for compound Naphthalene in sample Dec2818.D to y = 176, new integration is from x, y = 5.966, 176 to 6.003, 176 and new response = 121070; previous integration is from x, y = 5.966, 176 to 6.003, 5750 and previous response = 114805.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:12:26 AM	Set UserAnnotation = BA for compound Naphthalene in sample Dec2818.D; previous value =			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 9:12:31 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Dec2818.D, from x, y = 5.966, 350 to 6.003, 466, result = 20981; previous integration is from x, y = 5.938, 275 to 6.066, 275 and previous response = 29444.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 9:12:33 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Dec2818.D to y = 350, new integration is from x, y = 5.966, 350 to 6.003, 350 and new response = 21111; previous integration is from x, y = 5.966, 350 to 6.003, 466 and previous response = 20981.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 9:12:48 AM	Manually integrate qualifier 115.0 of compound 1-Methylnaphthalene in sample Dec2818.D, from x, y = 6.902, 1784 to 6.952, 1827, result = 19670; previous integration is from x, y = 6.865, 287 to 6.952, 287 and previous response = 28710.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 9:13:01 AM	Manually integrate qualifier 128.0 of compound Nitrobenzene-d5 in sample Dec2818.D, from x, y = 5.156, 1565 to 5.243, 176, result = 5093; previous integration is from x, y = 5.118, 176 to 5.243, 176 and previous response = 9702.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 9:13:03 AM	Drop baseline for qualifier 128.0 of compound Nitrobenzene-d5 in sample Dec2818.D to y = 176, new integration is from x, y = 5.156, 176 to 5.243, 176 and new response = 8721; previous integration is from x, y = 5.156, 1565 to 5.243, 176 and previous response = 5093.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 9:13:07 AM	Manually integrate qualifier 54.0 of compound Nitrobenzene-d5 in sample Dec2818.D, from x, y = 5.168, 717 to 5.243, 858, result = 5720; previous integration is from x, y = 5.156, 293 to 5.255, 301 and previous response = 8093.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	12/29/2021 9:13:09 AM	Snap baseline for qualifier 54.0 of compound Nitrobenzene-d5 in sample Dec2818.D from x = 5.168 to x = 5.243, new integration is from x, y = 5.168, 375 to 5.243, 470 and new response = 7353; previous integration is from x, y = 5.168, 717 to 5.243, 858 and previous response = 5720.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 9:13:10 AM	Drop baseline for qualifier 54.0 of compound Nitrobenzene-d5 in sample Dec2818.D to y = 375, new integration is from x, y = 5.168, 375 to 5.243, 375 and new response = 7566; previous integration is from x, y = 5.168, 375 to 5.243, 470 and previous response = 7353.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	12/29/2021 9:13:24 AM	Snap baseline for qualifier 115.0 of compound 2-Methylnaphthalene in sample Dec2818.D from x = 6.777 to x = 6.865, new integration is from x, y = 6.777, 2130 to 6.865, 1082 and new response = 18557; previous integration is from x, y = 6.777, 287 to 6.865, 287 and previous response = 25475.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 9:13:25 AM	Drop baseline for qualifier 115.0 of compound 2-Methylnaphthalene in sample Dec2818.D to y = 1082, new integration is from x, y = 6.777, 1082 to 6.865, 1082 and new response = 21306; previous integration is from x, y = 6.777, 2130 to 6.865, 1082 and previous response = 18557.			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:13:36 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Dec2818.D			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 9:13:42 AM	Manually integrate qualifier 167.0 of compound Fluorene in sample Dec2818.D from x, y = 8.661, 296 to 8.711, 243; result = 306			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	12/29/2021 9:13:44 AM	Snap baseline for qualifier 167.0 of compound Fluorene in sample Dec2818.D from x = 8.661 to x = 8.711, new integration is from x, y = 8.661, 293 to 8.711, 236 and new response = 320; previous integration is from x, y = 8.661, 296 to 8.711, 243 and previous response = 306.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 9:13:44 AM	Drop baseline for qualifier 167.0 of compound Fluorene in sample Dec2818.D to y = 236, new integration is from x, y = 8.661, 236 to 8.711, 236 and new response = 406; previous integration is from x, y = 8.661, 293 to 8.711, 236 and previous response = 320.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 9:13:54 AM	Manually integrate qualifier 167.0 of compound Fluorene in sample Dec2818.D, from x, y = 8.661, 297 to 8.698, 269, result = 252; previous integration is from x, y = 8.661, 236 to 8.711, 236 and previous response = 406.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 9:13:55 AM	Drop baseline for qualifier 167.0 of compound Fluorene in sample Dec2818.D to y = 269, new integration is from x, y = 8.661, 269 to 8.698, 269 and new response = 283; previous integration is from x, y = 8.661, 297 to 8.698, 269 and previous response = 252.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	12/29/2021 9:14:05 AM	Manually integrate qualifier 167.0 of compound Fluorene in sample Dec2818.D, from x, y = 8.661, 269 to 8.711, 309, result = 247; previous integration is from x, y = 8.661, 269 to 8.698, 269 and previous response = 283.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	12/29/2021 9:14:11 AM	Snap baseline for qualifier 167.0 of compound Fluorene in sample Dec2818.D from x = 8.661 to x = 8.711, new integration is from x, y = 8.661, 293 to 8.711, 236 and new response = 320; previous integration is from x, y = 8.661, 269 to 8.711, 309 and previous response = 247.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 9:14:12 AM	Drop baseline for qualifier 167.0 of compound Fluorene in sample Dec2818.D to y = 236, new integration is from x, y = 8.661, 236 to 8.711, 236 and new response = 406; previous integration is from x, y = 8.661, 293 to 8.711, 236 and previous response = 320.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	12/29/2021 9:14:19 AM	Manually integrate compound Chrysene in sample Dec2818.D, from x, y = 14.801, 215 to 14.851, 67, result = 21; previous integration is from x, y = 14.694, 67 to 14.851, 67 and previous response = 3364.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 9:14:20 AM	Drop baseline for compound Chrysene in sample Dec2818.D to y = 67, new integration is from x, y = 14.801, 67 to 14.851, 67 and new response = 241; previous integration is from x, y = 14.801, 215 to 14.851, 67 and previous response = 21.			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:14:24 AM	Zero out primary peak of compound Chrysene in sample Dec2818.D			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:14:27 AM	Zero out primary peak of compound Acenaphthylene in sample Dec2818.D			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:14:29 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Dec2818.D			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:14:45 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Dec2819.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegratePeak	BL2000\jheine	12/29/2021 9:14:50 AM	Manually integrate compound Acenaphthene in sample Dec2819.D, from x, y = 8.050, 280 to 8.113, 80, result = -240; previous integration is from x, y = 7.999, 80 to 8.113, 80 and previous response = 2564.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 9:14:52 AM	Drop baseline for compound Acenaphthene in sample Dec2819.D to y = 80, new integration is from x, y = 8.050, 80 to 8.113, 80 and new response = 134; previous integration is from x, y = 8.050, 280 to 8.113, 80 and previous response = -240.			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:14:54 AM	Zero out primary peak of compound Acenaphthene in sample Dec2819.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	12/29/2021 9:15:00 AM	Manually integrate compound Chrysene in sample Dec2819.D, from x, y = 14.801, 366 to 14.901, 59, result = -382; previous integration is from x, y = 14.691, 59 to 14.901, 59 and previous response = 3798.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 9:15:01 AM	Drop baseline for compound Chrysene in sample Dec2819.D to y = 59, new integration is from x, y = 14.801, 59 to 14.901, 59 and new response = 535; previous integration is from x, y = 14.801, 366 to 14.901, 59 and previous response = -382.			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:15:07 AM	Zero out primary peak of compound Chrysene in sample Dec2819.D			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:15:10 AM	Zero out primary peak of compound Fluorene in sample Dec2819.D			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:15:12 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Dec2819.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	12/29/2021 9:15:32 AM	Manually integrate compound Benzo(a)pyrene in sample Dec2820.D, from x, y = 18.289, 1483 to 18.289, 1500, result = 0; previous integration is from x, y = 18.476, 98 to 18.586, 104 and previous response = 2541.			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:15:33 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Dec2820.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	12/29/2021 9:15:40 AM	Manually integrate compound Acenaphthene in sample Dec2820.D, from x, y = 8.050, 321 to 8.113, 79, result = -343; previous integration is from x, y = 8.000, 79 to 8.113, 79 and previous response = 2167.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 9:15:42 AM	Drop baseline for compound Acenaphthene in sample Dec2820.D to y = 79, new integration is from x, y = 8.050, 79 to 8.113, 79 and new response = 109; previous integration is from x, y = 8.050, 321 to 8.113, 79 and previous response = -343.			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:15:44 AM	Zero out primary peak of compound Acenaphthene in sample Dec2820.D			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:15:47 AM	Zero out primary peak of compound Chrysene in sample Dec2820.D			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:15:49 AM	Zero out primary peak of compound Fluorene in sample Dec2820.D			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:15:51 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Dec2820.D			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:16:04 AM	Zero out primary peak of compound Fluorene in sample Dec2821.D			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:16:07 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Dec2821.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	12/29/2021 9:16:13 AM	Manually integrate compound Acenaphthene in sample Dec2821.D, from x, y = 8.050, 331 to 8.107, 110, result = -275; previous integration is from x, y = 7.994, 110 to 8.107, 110 and previous response = 2834.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 9:16:14 AM	Drop baseline for compound Acenaphthene in sample Dec2821.D to y = 110, new integration is from x, y = 8.050, 110 to 8.107, 110 and new response = 97; previous integration is from x, y = 8.050, 331 to 8.107, 110 and previous response = -275.			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:16:16 AM	Zero out primary peak of compound Acenaphthene in sample Dec2821.D			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:16:19 AM	Zero out primary peak of compound Chrysene in sample Dec2821.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	12/29/2021 9:16:30 AM	Manually integrate compound Acenaphthylene in sample Dec2821.D, from x, y = 7.826, 138 to 7.888, 142, result = 158; previous integration is from x, y = 7.965, 144 to 8.113, 146 and previous response = 1546.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	12/29/2021 9:16:33 AM	Manually integrate compound Acenaphthylene in sample Dec2821.D, from x, y = 7.838, 142 to 7.888, 142, result = 114; previous integration is from x, y = 7.826, 138 to 7.888, 142 and previous response = 158.			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:16:34 AM	Zero out primary peak of compound Acenaphthylene in sample Dec2821.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:16:37 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Dec2821.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	12/29/2021 9:16:54 AM	Manually integrate compound Benzo(a)pyrene in sample Dec2822.D, from x, y = 18.376, 91 to 18.425, 115, result = 142; previous integration is from x, y = 18.462, 96 to 18.598, 118 and previous response = 2688.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 9:16:56 AM	Drop baseline for compound Benzo(a)pyrene in sample Dec2822.D to y = 91, new integration is from x, y = 18.376, 91 to 18.425, 91 and new response = 178; previous integration is from x, y = 18.376, 91 to 18.425, 115 and previous response = 142.			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:16:57 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Dec2822.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	12/29/2021 9:17:03 AM	Manually integrate compound Acenaphthene in sample Dec2822.D, from x, y = 8.050, 143 to 8.113, 81, result = 158; previous integration is from x, y = 8.001, 81 to 8.113, 81 and previous response = 2320.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 9:17:04 AM	Drop baseline for compound Acenaphthene in sample Dec2822.D to y = 81, new integration is from x, y = 8.050, 81 to 8.113, 81 and new response = 275; previous integration is from x, y = 8.050, 143 to 8.113, 81 and previous response = 158.			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:17:06 AM	Zero out primary peak of compound Acenaphthene in sample Dec2822.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	12/29/2021 9:17:12 AM	Manually integrate compound Chrysene in sample Dec2822.D, from x, y = 14.789, 220 to 14.888, 182, result = -229; previous integration is from x, y = 14.690, 59 to 14.789, 59 and previous response = 2986.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	12/29/2021 9:17:14 AM	Snap baseline for compound Chrysene in sample Dec2822.D, from x = 14.789 to x = 14.888, new integration is from x, y = 14.789, 155 to 14.888, 88 and new response = 245; previous integration is from x, y = 14.789, 220 to 14.888, 182 and previous response = -229.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 9:17:15 AM	Drop baseline for compound Chrysene in sample Dec2822.D to y = 88, new integration is from x, y = 14.789, 88 to 14.888, 88 and new response = 445; previous integration is from x, y = 14.789, 155 to 14.888, 88 and previous response = 245.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:17:17 AM	Zero out primary peak of compound Chrysene in sample Dec2822.D			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:17:21 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Dec2822.D			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:17:38 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Dec2823.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	12/29/2021 9:17:45 AM	Manually integrate compound Acenaphthene in sample Dec2823.D, from x, y = 8.038, 168 to 8.113, 120, result = 308; previous integration is from x, y = 8.001, 120 to 8.113, 120 and previous response = 2621.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 9:17:47 AM	Drop baseline for compound Acenaphthene in sample Dec2823.D to y = 120, new integration is from x, y = 8.038, 120 to 8.113, 120 and new response = 416; previous integration is from x, y = 8.038, 168 to 8.113, 120 and previous response = 308.			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:17:48 AM	Zero out primary peak of compound Acenaphthene in sample Dec2823.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	12/29/2021 9:17:58 AM	Manually integrate compound Naphthalene in sample Dec2823.D, from x, y = 5.966, 187 to 6.003, 357, result = 549; previous integration is from x, y = 5.966, 187 to 6.078, 208 and previous response = 3333.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 9:17:59 AM	Drop baseline for compound Naphthalene in sample Dec2823.D to y = 187, new integration is from x, y = 5.966, 187 to 6.003, 187 and new response = 741; previous integration is from x, y = 5.966, 187 to 6.003, 357 and previous response = 549.			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:18:00 AM	Zero out primary peak of compound Naphthalene in sample Dec2823.D			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:18:04 AM	Zero out primary peak of compound 1-Methylnaphthalene in sample Dec2823.D			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:18:07 AM	Zero out primary peak of compound Chrysene in sample Dec2823.D			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:18:09 AM	Zero out primary peak of compound 2-Methylnaphthalene in sample Dec2823.D			✓	
CmdZeroOutPeak	BL2000\jheine	12/29/2021 9:18:10 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Dec2823.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegratePeak	BL2000\jheine	12/29/2021 9:18:45 AM	Manually integrate compound Acenaphthene in sample Dec2824.D, from x, y = 8.038, 3410 to 8.150, 109, result = 12136; previous integration is from x, y = 8.001, 114 to 8.150, 109 and previous response = 24964.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	12/29/2021 9:18:46 AM	Drop baseline for compound Acenaphthene in sample Dec2824.D to y = 109, new integration is from x, y = 8.038, 109 to 8.150, 109 and new response = 23240; previous integration is from x, y = 8.038, 3410 to 8.150, 109 and previous response = 12136.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	12/29/2021 9:18:48 AM	Set UserAnnotation = CO for compound Acenaphthene in sample Dec2824.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:19:31 AM	Set SampleType = CC for sample Dec2824.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:19:39 AM	Set LevelName = CCV for sample Dec2824.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:19:49 AM	Set SampleType = Blank for sample Dec2811.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:19:54 AM	Set SampleType = Blank for sample Dec2812.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:20:00 AM	Set SampleType = Matrix for sample Dec2813.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:20:07 AM	Set SampleType = Matrix for sample Dec2814.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:20:13 AM	Set SampleType = MatrixDup for sample Dec2815.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:20:19 AM	Set MatrixSpikeGroup = MB-162432 for sample Dec2811.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:20:23 AM	Set MatrixSpikeGroup = MB-162432 for sample Dec2813.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:20:26 AM	Set MatrixSpikeGroup = MB-162432 for sample Dec2814.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:20:30 AM	Set MatrixSpikeGroup = MB-162432 for sample Dec2815.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:20:36 AM	Set MatrixSpikeGroup = for sample Dec2814.D; previous value = MB-162432			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:20:41 AM	Set SampleInformation = MatrixA for sample Dec2813.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:20:49 AM	Set SampleInformation = MatrixA for sample Dec2815.D; previous value =			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdQuantitate	BL2000\jheine	12/29/2021 9:21:01 AM	Quantitate all compounds in all samples			✓	
CmdSaveBatchTable	BL2000\jheine	12/29/2021 9:23:55 AM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh 122821\1_e8270c_bna SIM\QuantResults\122821_bna SIM 1.batch.bin			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:24:02 AM	Set SampleApproved = True for sample Dec2801.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:24:03 AM	Set SampleApproved = True for sample Dec2802.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:24:09 AM	Set SampleApproved = True for sample Dec2803.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:24:11 AM	Set SampleApproved = True for sample Dec2804.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:24:13 AM	Set SampleApproved = True for sample Dec2805.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:24:14 AM	Set SampleApproved = True for sample Dec2806.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:24:17 AM	Set SampleApproved = True for sample Dec2807.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:24:19 AM	Set SampleApproved = True for sample Dec2808.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:24:21 AM	Set SampleApproved = True for sample Dec2809.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:24:23 AM	Set SampleApproved = True for sample Dec2810.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:24:24 AM	Set SampleApproved = True for sample Dec2811.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:24:26 AM	Set SampleApproved = True for sample Dec2812.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:24:28 AM	Set SampleApproved = True for sample Dec2813.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:24:30 AM	Set SampleApproved = True for sample Dec2814.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:24:31 AM	Set SampleApproved = True for sample Dec2815.D; previous value = False			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:24:33 AM	Set SampleApproved = True for sample Dec2816.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:24:34 AM	Set SampleApproved = True for sample Dec2817.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:24:36 AM	Set SampleApproved = True for sample Dec2818.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:24:38 AM	Set SampleApproved = True for sample Dec2819.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:24:40 AM	Set SampleApproved = True for sample Dec2820.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:24:41 AM	Set SampleApproved = True for sample Dec2821.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:24:43 AM	Set SampleApproved = True for sample Dec2822.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:24:45 AM	Set SampleApproved = True for sample Dec2823.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	12/29/2021 9:24:46 AM	Set SampleApproved = True for sample Dec2824.D; previous value = False			✓	
CmdSaveBatchTable	BL2000\jheine	12/29/2021 9:24:50 AM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\QuantResults\122821 bna SIM 1.batch.bin			✓	
CmdOpenBatchTable	BL2000\jheine	12/29/2021 4:26:08 PM	Open batch \\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\122821 bna SIM 1.batch.bin			✓	
CmdSaveBatchTable	BL2000\jheine	12/29/2021 5:14:09 PM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\QuantResults\122821 bna SIM 1.batch.bin			✓	
CmdOpenBatchTable	BL2000\jheine	1/6/2022 12:19:30 PM	Open batch \\MASSHUNTER\Org\Data\SV5975.I\Old Data\2021 Data\sh122821\1 e8270c bna SIM\122821 bna SIM 1.batch.bin			✓	
GenerateReport	BL2000\jheine	1/6/2022 12:26:40 PM	Generates report - Method: D:\Org\reports\GCMSSEMI Report Templates\Calibration\Gen_Calibration.m, Output Path: \\MASSHUNTER\Org\Data\SV5975.I\Old Data\2021 Data\sh122821\1 e8270c bna SIM\QuantReports\			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
GenerateReport	BL2000\jheine	1/6/2022 12:27:42 PM	Generates report - Method: D:\Org\reports\GCMSSSEMI Report Templates\Calibration\init_cal_rpt.m, Output Path: \\MASSHUNTER\Org\Data\SV5975.I\Old Data\2021 Data\sh122821\1 e8270c bna SIM\QuantReports\			✓	
GenerateReport	BL2000\jheine	1/6/2022 12:28:42 PM	Generates report - Method: D:\Org\reports\GCMSSSEMI Report Templates\Calibration\Gen_ResultsSummary.m, Output Path: \\MASSHUNTER\Org\Data\SV5975.I\Old Data\2021 Data\sh122821\1 e8270c bna SIM\QuantReports\			✓	
GenerateReport	BL2000\jheine	1/6/2022 12:29:55 PM	Generates report - Method: D:\Org\reports\GCMSSSEMI Report Templates\Calibration\Env_QuantResults_wGraphics+Chromatogram.m, Output Path: \\MASSHUNTER\Org\Data\SV5975.I\Old Data\2021 Data\sh122821\1 e8270c bna SIM\QuantReports\				Agilent.MassSpectrometry.DataAnalysis.Quantitative.ApplicationCommandCancelledException: Generating report(s) was canceled by user. at Agilent.MassSpectrometry.DataAnalysis.Quantitative.GenerateReport.RunReportMethod(ICompliance compliance, String user, String batchFolder, String batchFile, String method, String outputPath, String applicationType, String cancelEventName, Int16[] samples, Int16[] compounds, String logonXml, Action `1 progress) at Agilent.MassSpectrometry.DataAnalysis.Quantitative.GenerateReport.Do() at Agilent.MassSpectrometry.CommandModel.CommandHistory.Invoke(ICommand cmd) at Agilent.MassSpectrometry.DataAnalysis.Quantitative.AppCommandContext._Invoke(ICommand cmd)
GenerateReport	BL2000\jheine	1/6/2022 12:33:34 PM	Generates report - Method: D:\Org\reports\GCMSSSEMI Report Templates\Calibration\Env_QuantResults_wGraphics+Chromatogram.m, Output Path: \\MASSHUNTER\Org\Data\SV5975.I\Old Data\2021 Data\sh122821\1 e8270c bna SIM\QuantReports\			✓	

Energy Laboratories Inc

ANALYTICAL RUN Summary

24-Feb-22

Run ID SV5975.I_220110A

Run Start Date: 1/10/2022
Analyst: John P. Heine
Ical:
Column ID: ZB-SemiVolatiles
Comments:

Std ID	Std Name	Std Amount	Std Units	Samp Amount	Samp Units	SampType	Expiration Date
dcmsvoc13	DCM						11/17/2022
sv100210	BNA 2nd source 200ug/mL	2	ul	198	ul	ICV	1/15/2022
sv100506	BNA low 50 ug/mL	8	ul	192	ul	CCV	3/31/2022
sv100703	BNA Internals 2000 ug/mL	2	ul	100	ul	SAMP	5/31/2022
sv83311	DFTPP 1000 ug/mL	50	ul	50	ul	TUNE	10/31/2022

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14972033	Jan1001_D_TU	SVOC-8270-DF	TUNE	√5975.I\sh0110221	1/10/2022 11:19:	1	R372987		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
127, % of mass 198	A	%	52.8	52.8		100	0	0	0	0.01	0	53%	40	60	0%	
197, % of mass 198	A	%	0	0		100	0	0	0	0.01	0	0%	0	0.99	0%	
198, Base Peak	A	%	100	100		100	0	0	0	0.01	0	100%	100	100	0%	
199, % of mass 198	A	%	7.1	7.1		100	0	0	0	0.01	0	7%	5	9	0%	
275, % of mass 198	A	%	29.5	29.5		100	0	0	0	0.01	0	30%	10	30	0%	
365, % of mass 198	A	%	3.7	3.7		100	0	0	0	0.01	0	4%	1	99.99	0%	
441, % of mass 443	A	%	89.9	89.9		100	0	0	0	0.01	0	90%	0.01	150	0%	
442, % of mass 198	A	%	80.7	80.7		100	0	0	0	0.01	0	81%	40	100	0%	
443, % of mass 442	A	%	19.2	19.2		100	0	0	0	0.01	0	19%	17	23	0%	
51, % of mass 198	A	%	46.9	46.9		100	0	0	0	0.01	0	47%	30	60	0%	
68, % of mass 69	A	%	0	0		100	0	0	0	0.01	0	0%	0	1.99	0%	
70, % of mass 69	A	%	0.5	0.5		100	0	0	0	0.01	0	1%	0	1.99	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14972035	10-Jan-22_CC	SVOC-8270-W-	CCV	√5975.I\sh0110221	10/2022 11:43:	1	R372987		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	2.15763	2.15763		2	0	0	0.0206	0.1	10	108%	80	120	0%	
2-Methylnaphthalene	A	ug/L	1.87353	1.87353		2	0	0	0.0176	0.1	10	94%	80	120	0%	
Naphthalene	A	ug/L	1.90328	1.90328		2	0	0	0.029	0.1	10	95%	80	120	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
2-Fluorobiphenyl	S	ug/L	1.92679	1.92679		2	0	0	0.0444	0.1	10	96%	80	120	0%	
Nitrobenzene-d5	S	ug/L	1.70463	1.70463		2	0	0	0.0523	0.1	10	85%	80	120	0%	
Terphenyl-d14	S	ug/L	1.96182	1.96182		2	0	0	0.0563	0.1	10	98%	80	120	0%	
o-Terphenyl	X	ug/L	1.78408	1.78408		2	0	0	0.0654	0.1	10	89%	80	120	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14972036	10-Jan-22_ISTB	SVOC-8270-W-	SAMP	√5975.I\sh0110221	10/2022 12:15:	1	R372987		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0206	0.1	10	0%	0	0	0%	
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0176	0.1	10	0%	0	0	0%	
Acenaphthene	A	ug/L	0	0		0	0	0	0.0317	0.1	10	0%	0	0	0%	
Acenaphthylene	A	ug/L	0	0		0	0	0	0.025	0.1	10	0%	0	0	0%	
Anthracene	A	ug/L	0	0		0	0	0	0.0283	0.1	10	0%	0	0	0%	
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.0272	0.1	10	0%	0	0	0%	
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.0347	0.1	10	0%	0	0	0%	
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.0226	0.1	10	0%	0	0	0%	
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.0267	0.1	10	0%	0	0	0%	
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.0295	0.1	10	0%	0	0	0%	
Chrysene	A	ug/L	0	0		0	0	0	0.0458	0.1	10	0%	0	0	0%	
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.0367	0.1	10	0%	0	0	0%	
Fluoranthene	A	ug/L	0	0		0	0	0	0.0233	0.1	10	0%	0	0	0%	
Fluorene	A	ug/L	0	0		0	0	0	0.0225	0.1	10	0%	0	0	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.0491	0.1	10	0%	0	0	0%	
Naphthalene	A	ug/L	0	0		0	0	0	0.029	0.1	10	0%	0	0	0%	
Phenanthrene	A	ug/L	0	0		0	0	0	0.0295	0.1	10	0%	0	0	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14972036	10-Jan-22_ISTB	SVOC-8270-W-	SAMP	√5975.I\sh0110221	10/2022 12:15:	1	R372987		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Pyrene	A	ug/L	0	0		0	0	0	0.0239	0.1	10	0%	0	0	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
2-Fluorobiphenyl	S	ug/L	0	0		5	0	0	0.0444	0.1	10	0%	25	94	0%	S
Nitrobenzene-d5	S	ug/L	0	0		5	0	0	0.0523	0.1	10	0%	19	102	0%	S
Terphenyl-d14	S	ug/L	0	0		5	0	0	0.0563	0.1	10	0%	39	106	0%	S
o-Terphenyl	X	ug/L	0	0		200	0	0	0.0654	0.1	10	0%	40	140	0%	S

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14972037	MB-162577	SVOC-8270-W-	MBLK	√5975.I\sh0110221	10/2022 12:48:	1	162577	12/29/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0206	0.1	10	0%			0%	
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0176	0.1	10	0%			0%	
Naphthalene	A	ug/L	0	0		0	0	0	0.029	0.1	10	0%			0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14972038	MB-162577	SVOC-8270-W-	MBLK	√5975.I\sh0110221	10/2022 1:20:2	20	162577	12/29/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
2-Fluorobiphenyl	S	ug/L	2.13744	42.7488		100	0	0	0.888	2	10	43%	53	106	0%	S
Nitrobenzene-d5	S	ug/L	2.95212	59.0424		100	0	0	1.046	2	10	59%	55	111	0%	
Terphenyl-d14	S	ug/L	4.81802	96.3604		100	0	0	1.126	2	10	96%	58	132	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14972039	LLCS-162577	SVOC-8270-W-	LCS-DOD	√5975.I\sh0110221	10/2022 1:53:0	1	162577	12/29/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	3.13854	3.13854		5	0	0	0.0206	0.1	10	63%	41	115	0%	
2-Methylnaphthalene	A	ug/L	3.01302	3.01302		5	0	0	0.0176	0.1	10	60%	39	114	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14972039	LLCS-162577	SVOC-8270-W-	LCS-DOD	√5975.I\sh0110221	10/2022 1:53:0	1	162577	12/29/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Naphthalene	A	ug/L	2.84952	2.84952		5	0	0	0.029	0.1	10	57%	43	114	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
2-Fluorobiphenyl	S	ug/L	3.75008	3.75008		5	0	0	0.0444	0.1	10	75%	53	106	0%	
Nitrobenzene-d5	S	ug/L	3.45553	3.45553		5	0	0	0.0523	0.1	10	69%	55	111	0%	
Terphenyl-d14	S	ug/L	5.01046	5.01046		5	0	0	0.0563	0.1	10	100%	58	132	0%	
o-Terphenyl	X	ug/L	4.08365	4.08365		5	0	0	0.0654	0.1	10	82%	40	140	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14972040	LLCSD-162577	SVOC-8270-W-	LCS-DOD	√5975.I\sh0110221	10/2022 2:25:2	1	162577	12/29/2021	0	1E+07						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	2.92236	2.92236		5	0	3.13854	0.0206	0.1	10	58%	41	115	7%	
2-Methylnaphthalene	A	ug/L	2.84818	2.84818		5	0	3.01302	0.0176	0.1	10	57%	39	114	6%	
Naphthalene	A	ug/L	2.43305	2.43305		5	0	2.84952	0.029	0.1	10	49%	43	114	16%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
2-Fluorobiphenyl	S	ug/L	3.72519	3.72519		5	0	0	0.0444	0.1	10	75%	53	106	0%	
Nitrobenzene-d5	S	ug/L	3.7783	3.7783		5	0	0	0.0523	0.1	10	76%	55	111	0%	
Terphenyl-d14	S	ug/L	5.27057	5.27057		5	0	0	0.0563	0.1	10	105%	58	132	0%	
o-Terphenyl	X	ug/L	4.33768	4.33768		5	0	4.08365	0.0654	0.1	10	87%	40	140	6%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14972041	B21122077-001	SVOC-8270-W-	SAMP	√5975.I\sh0110221	10/2022 2:57:5	1	162577	12/29/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14972041	B21122077-001	SVOC-8270-W-	SAMP	√5975.I\sh0110221	10/2022 2:57:5	1	162577	12/29/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.020188	0.1	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.017248	0.1	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.02842	0.1	10	0%	0	0	0%	U
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14972042	B21122077-001	SVOC-8270-W-	SAMP	√5975.I\sh0110221	10/2022 3:30:1	20	162577	12/29/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
2-Fluorobiphenyl	S	ug/L	3.21814	63.075544		98	0	0	0.87024	1.96	10	64%	53	106	0%	
Nitrobenzene-d5	S	ug/L	2.89251	56.693196		98	0	0	1.02508	1.96	10	58%	55	111	0%	
Terphenyl-d14	S	ug/L	4.68118	91.751128		98	0	0	1.10348	1.96	10	94%	58	132	0%	
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14972043	B21122088-001	SVOC-8270-W-	SAMP	√5975.I\sh0110221	10/2022 4:02:4	1	162577	12/29/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.02163	0.105	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.01848	0.105	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.03045	0.105	10	0%	0	0	0%	U
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14972044	B21122088-001	SVOC-8270-W-	SAMP	√5975.I\sh0110221	10/2022 4:35:0	20	162577	12/29/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
2-Fluorobiphenyl	S	ug/L	3.05554	64.16634		105	0	0	0.9324	2.1	10	61%	53	106	0%	
Nitrobenzene-d5	S	ug/L	3.13907	65.92047		105	0	0	1.0983	2.1	10	63%	55	111	0%	
Terphenyl-d14	S	ug/L	5.18366	108.85686		105	0	0	1.1823	2.1	10	104%	58	132	0%	
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14972045	B21122090-001	SVOC-8270-W-	SAMP	√5975.I\sh0110221	10/2022 5:07:2	1	162577	12/29/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14972045	B21122090-001	SVOC-8270-W-	SAMP	√5975.I\sh0110221	10/2022 5:07:2	1	162577	12/29/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0206	0.1	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0176	0.1	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.029	0.1	10	0%	0	0	0%	U
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14972046	B21122090-001	SVOC-8270-W-	SAMP	√5975.I\sh0110221	10/2022 5:39:4	20	162577	12/29/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
2-Fluorobiphenyl	S	ug/L	3.24818	64.9636		100	0	0	0.888	2	10	65%	53	106	0%	
Nitrobenzene-d5	S	ug/L	2.59194	51.8388		100	0	0	1.046	2	10	52%	55	111	0%	S
Terphenyl-d14	S	ug/L	4.85337	97.0674		100	0	0	1.126	2	10	97%	58	132	0%	
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14972047	B21122105-001	SVOC-8270-W-	SAMP	√5975.I\sh0110221	10/2022 6:12:0	1	162577	12/29/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0198172	0.1	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0169312	0.1	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.027898	0.1	10	0%	0	0	0%	U
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14972048	B21122105-001	SVOC-8270-W-	SAMP	√5975.I\sh0110221	10/2022 6:44:2	20	162577	12/29/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
2-Fluorobiphenyl	S	ug/L	3.59346	69.1381704		96.2	0	0	0.854256	1.924	10	72%	53	106	0%	
Nitrobenzene-d5	S	ug/L	3.1714	61.017736		96.2	0	0	1.006252	1.924	10	63%	55	111	0%	
Terphenyl-d14	S	ug/L	5.17416	99.5508384		96.2	0	0	1.083212	1.924	10	103%	58	132	0%	
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14972049	B21122105-001	SVOC-8270-W-	MS-DOD	√5975.I\sh0110221	10/2022 7:16:5	1	162577	12/29/2021	1E+07	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14972049	B21122105-001	SVOC-8270-W-	MS-DOD	√5975.I\sh0110221	10/2022 7:16:5	1	162577	12/29/2021	1E+07	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	3.78436	3.78436		5	0	0	0.0206	0.1	10	76%	41	115	0%	
2-Methylnaphthalene	A	ug/L	3.60519	3.60519		5	0	0	0.0176	0.1	10	72%	39	114	0%	
Naphthalene	A	ug/L	3.28255	3.28255		5	0	0	0.029	0.1	10	66%	43	114	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
2-Fluorobiphenyl	S	ug/L	3.941	3.941		5	0	0	0.0444	0.1	10	79%	53	106	0%	
Nitrobenzene-d5	S	ug/L	3.09846	3.09846		5	0	0	0.0523	0.1	10	62%	55	111	0%	
Terphenyl-d14	S	ug/L	5.11748	5.11748		5	0	0	0.0563	0.1	10	102%	58	132	0%	
o-Terphenyl	X	ug/L	4.32186	4.32186		5	0	0	0.0654	0.1	10	86%	40	140	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14972050	MB-162701	SVOC-8270-W-	MBLK	√5975.I\sh0110221	10/2022 7:49:1	1	162701	1/4/2022 3:4	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0206	0.1	10	0%			0%	
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0176	0.1	10	0%			0%	
Acenaphthene	A	ug/L	0	0		0	0	0	0.0317	0.1	10	0%			0%	
Acenaphthylene	A	ug/L	0	0		0	0	0	0.025	0.1	10	0%			0%	
Anthracene	A	ug/L	0	0		0	0	0	0.0283	0.1	10	0%			0%	
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.0272	0.1	10	0%			0%	
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.0347	0.1	10	0%			0%	
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.0226	0.1	10	0%			0%	
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.0267	0.1	10	0%			0%	
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.0295	0.1	10	0%			0%	
Chrysene	A	ug/L	0	0		0	0	0	0.0458	0.1	10	0%			0%	
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.0367	0.1	10	0%			0%	
Fluoranthene	A	ug/L	0	0		0	0	0	0.0233	0.1	10	0%			0%	
Fluorene	A	ug/L	0	0		0	0	0	0.0225	0.1	10	0%			0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.0491	0.1	10	0%			0%	
Naphthalene	A	ug/L	0	0		0	0	0	0.029	0.1	10	0%			0%	
Phenanthrene	A	ug/L	0	0		0	0	0	0.0295	0.1	10	0%			0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14972050	MB-162701	SVOC-8270-W-	MBLK	√5975.I\sh0110221	10/2022 7:49:1	1	162701	1/4/2022 3:4	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Pyrene	A	ug/L	0	0		0	0	0	0.0239	0.1	10	0%			0%	
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14972051	MB-162701	SVOC-8270-W-	MBLK	√5975.I\sh0110221	10/2022 8:21:3	20	162701	1/4/2022 3:4	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
2-Fluorobiphenyl	S	ug/L	3.20926	64.1852		100	0	0	0.888	2	10	64%	53	106	0%	
Nitrobenzene-d5	S	ug/L	3.14184	62.8368		100	0	0	1.046	2	10	63%	55	111	0%	
Terphenyl-d14	S	ug/L	4.85091	97.0182		100	0	0	1.126	2	10	97%	58	132	0%	
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14972052	LLCS-162701	SVOC-8270-W-	LCS-DOD	√5975.I\sh0110221	10/2022 8:53:5	1	162701	1/4/2022 3:4	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	3.82578	3.82578		5	0	0	0.0206	0.1	10	77%	41	115	0%	
2-Methylnaphthalene	A	ug/L	3.61943	3.61943		5	0	0	0.0176	0.1	10	72%	39	114	0%	
Acenaphthene	A	ug/L	3.55205	3.55205		5	0	0	0.0317	0.1	10	71%	48	114	0%	
Acenaphthylene	A	ug/L	3.77187	3.77187		5	0	0	0.025	0.1	10	75%	35	121	0%	
Anthracene	A	ug/L	4.47355	4.47355		5	0	0	0.0283	0.1	10	89%	53	119	0%	
Benzo(a)anthracene	A	ug/L	4.38375	4.38375		5	0	0	0.0272	0.1	10	88%	59	120	0%	
Benzo(a)pyrene	A	ug/L	4.00927	4.00927		5	0	0	0.0347	0.1	10	80%	53	120	0%	
Benzo(b)fluoranthene	A	ug/L	4.03231	4.03231		5	0	0	0.0226	0.1	10	81%	53	126	0%	
Benzo(g,h,i)perylene	A	ug/L	4.24138	4.24138		5	0	0	0.0267	0.1	10	85%	44	128	0%	
Benzo(k)fluoranthene	A	ug/L	4.16296	4.16296		5	0	0	0.0295	0.1	10	83%	54	125	0%	
Chrysene	A	ug/L	4.48354	4.48354		5	0	0	0.0458	0.1	10	90%	57	120	0%	
Dibenzo(a,h)anthracene	A	ug/L	4.18259	4.18259		5	0	0	0.0367	0.1	10	84%	44	141	0%	
Fluoranthene	A	ug/L	4.02741	4.02741		5	0	0	0.0233	0.1	10	81%	58	120	0%	
Fluorene	A	ug/L	4.06961	4.06961		5	0	0	0.0225	0.1	10	81%	50	118	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	4.01732	4.01732		5	0	0	0.0491	0.1	10	80%	48	130	0%	
Naphthalene	A	ug/L	3.44371	3.44371		5	0	0	0.029	0.1	10	69%	43	114	0%	
Phenanthrene	A	ug/L	4.20217	4.20217		5	0	0	0.0295	0.1	10	84%	53	115	0%	
Pyrene	A	ug/L	4.02576	4.02576		5	0	0	0.0239	0.1	10	81%	53	121	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14972052	LLCS-162701	SVOC-8270-W-	LCS-DOD	√5975.I\sh0110221	10/2022 8:53:5	1	162701	1/4/2022 3:4	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%				0%
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%				0%
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%				0%
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%				0%
2-Fluorobiphenyl	S	ug/L	3.74398	3.74398		5	0	0	0.0444	0.1	10	75%	53	106		0%
Nitrobenzene-d5	S	ug/L	3.40025	3.40025		5	0	0	0.0523	0.1	10	68%	55	111		0%
Terphenyl-d14	S	ug/L	4.60733	4.60733		5	0	0	0.0563	0.1	10	92%	58	132		0%
o-Terphenyl	X	ug/L	3.85555	3.85555		5	0	0	0.0654	0.1	10	77%	40	140		0%

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14972053	LLCSD-162701	SVOC-8270-W-	LCSD-DOD	√5975.I\sh0110221	10/2022 9:26:2	1	162701	1/4/2022 3:4	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	3.88411	3.88411		5	0	0	0.0206	0.1	10	78%	41	115		0%
2-Methylnaphthalene	A	ug/L	3.69507	3.69507		5	0	0	0.0176	0.1	10	74%	39	114		0%
Acenaphthene	A	ug/L	3.79029	3.79029		5	0	0	0.0317	0.1	10	76%	48	114		0%
Acenaphthylene	A	ug/L	3.96129	3.96129		5	0	0	0.025	0.1	10	79%	35	121		0%
Anthracene	A	ug/L	4.54194	4.54194		5	0	0	0.0283	0.1	10	91%	53	119		0%
Benzo(a)anthracene	A	ug/L	4.4757	4.4757		5	0	0	0.0272	0.1	10	90%	59	120		0%
Benzo(a)pyrene	A	ug/L	3.98387	3.98387		5	0	0	0.0347	0.1	10	80%	53	120		0%
Benzo(b)fluoranthene	A	ug/L	3.93104	3.93104		5	0	0	0.0226	0.1	10	79%	53	126		0%
Benzo(g,h,i)perylene	A	ug/L	4.15901	4.15901		5	0	0	0.0267	0.1	10	83%	44	128		0%
Benzo(k)fluoranthene	A	ug/L	4.04506	4.04506		5	0	0	0.0295	0.1	10	81%	54	125		0%
Chrysene	A	ug/L	4.47689	4.47689		5	0	0	0.0458	0.1	10	90%	57	120		0%
Dibenzo(a,h)anthracene	A	ug/L	4.24952	4.24952		5	0	0	0.0367	0.1	10	85%	44	141		0%
Fluoranthene	A	ug/L	4.24824	4.24824		5	0	0	0.0233	0.1	10	85%	58	120		0%
Fluorene	A	ug/L	4.14584	4.14584		5	0	0	0.0225	0.1	10	83%	50	118		0%
Indeno(1,2,3-cd)pyrene	A	ug/L	4.03105	4.03105		5	0	0	0.0491	0.1	10	81%	48	130		0%
Naphthalene	A	ug/L	3.44292	3.44292		5	0	0	0.029	0.1	10	69%	43	114		0%
Phenanthrene	A	ug/L	4.23911	4.23911		5	0	0	0.0295	0.1	10	85%	53	115		0%
Pyrene	A	ug/L	4.12444	4.12444		5	0	0	0.0239	0.1	10	82%	53	121		0%
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%				0%
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%				0%
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%				0%
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%				0%

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14972053	LLCSD-162701	SVOC-8270-W-	LCSD-DOD	√5975.I\sh0110221	1/10/2022 9:26:2	1	162701	1/4/2022 3:4	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%				0%
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%				0%
2-Fluorobiphenyl	S	ug/L	3.80294	3.80294		5	0	0	0.0444	0.1	10	76%	53	106		0%
Nitrobenzene-d5	S	ug/L	3.02278	3.02278		5	0	0	0.0523	0.1	10	60%	55	111		0%
Terphenyl-d14	S	ug/L	4.71004	4.71004		5	0	0	0.0563	0.1	10	94%	58	132		0%
o-Terphenyl	X	ug/L	3.90641	3.90641		5	0	0	0.0654	0.1	10	78%	40	140		0%

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14972054	B22010096-001	SVOC-8270-W-	SAMP	√5975.I\sh0110221	1/10/2022 9:58:3	1	162701	1/4/2022 3:4	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.020188	0.1	10	0%	0	0		0% U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.017248	0.1	10	0%	0	0		0% U
Acenaphthene	A	ug/L	0	0		0	0	0	0.031066	0.1	10	0%	0	0		0% U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.0245	0.1	10	0%	0	0		0% U
Anthracene	A	ug/L	0	0		0	0	0	0.027734	0.1	10	0%	0	0		0% U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.026656	0.1	10	0%	0	0		0% U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.034006	0.1	10	0%	0	0		0% U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.022148	0.1	10	0%	0	0		0% U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.026166	0.1	10	0%	0	0		0% U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.02891	0.1	10	0%	0	0		0% U
Chrysene	A	ug/L	0	0		0	0	0	0.044884	0.1	10	0%	0	0		0% U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.035966	0.1	10	0%	0	0		0% U
Fluoranthene	A	ug/L	0	0		0	0	0	0.022834	0.1	10	0%	0	0		0% U
Fluorene	A	ug/L	0	0		0	0	0	0.02205	0.1	10	0%	0	0		0% U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.048118	0.1	10	0%	0	0		0% U
Naphthalene	A	ug/L	0	0		0	0	0	0.02842	0.1	10	0%	0	0		0% U
Phenanthrene	A	ug/L	0	0		0	0	0	0.02891	0.1	10	0%	0	0		0% U
Pyrene	A	ug/L	0	0		0	0	0	0.023422	0.1	10	0%	0	0		0% U

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14972055	B22010096-001	SVOC-8270-W-	SAMP	√5975.I\sh0110221	1/10/2022 10:31:	20	162701	1/4/2022 3:4	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14972055	B22010096-001	SVOC-8270-W-	SAMP	√5975.I\sh0110221	10/2022 10:31:	20	162701	1/4/2022 3:4	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
2-Fluorobiphenyl	S	ug/L	3.76435	73.78126		98	0	0	0.87024	1.96	10	75%	53	106	0%	
Nitrobenzene-d5	S	ug/L	3.2082	62.88072		98	0	0	1.02508	1.96	10	64%	55	111	0%	
Terphenyl-d14	S	ug/L	5.31803	104.233388		98	0	0	1.10348	1.96	10	106%	58	132	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14972056	10-Jan-22_CCV	SVOC-8270-W-	CCV	√5975.I\sh0110221	10/2022 11:03:	1	R372987		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	2.22886	2.22886		2	0	0	0.0206	0.1	10	111%	50	150	0%	
2-Methylnaphthalene	A	ug/L	1.96397	1.96397		2	0	0	0.0176	0.1	10	98%	50	150	0%	
Naphthalene	A	ug/L	1.86331	1.86331		2	0	0	0.029	0.1	10	93%	50	150	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%	50	150	0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%	50	150	0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	50	150	0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%	50	150	0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	50	150	0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%	50	150	0%	
2-Fluorobiphenyl	S	ug/L	1.87756	1.87756		2	0	0	0.0444	0.1	10	94%	50	150	0%	
Nitrobenzene-d5	S	ug/L	1.68113	1.68113		2	0	0	0.0523	0.1	10	84%	50	150	0%	
Terphenyl-d14	S	ug/L	1.99684	1.99684		2	0	0	0.0563	0.1	10	100%	50	150	0%	
o-Terphenyl	X	ug/L	1.73962	1.73962		2	0	0	0.0654	0.1	10	87%	50	150	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14974167	10-Jan-22_CCV	SVOC-8270C-SI	CCV	√5975.I\sh0110221	10/2022 11:43:	1	R372987		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	2.15763	2.15763		2	0	0	0.0206	0.1	10	108%	80	120	0%	
2-Methylnaphthalene	A	ug/L	1.87353	1.87353		2	0	0	0.0176	0.1	10	94%	80	120	0%	
Acenaphthene	A	ug/L	1.80853	1.80853		2	0	0	0.0317	0.1	10	90%	80	120	0%	
Acenaphthylene	A	ug/L	1.97289	1.97289		2	0	0	0.025	0.1	10	99%	80	120	0%	
Anthracene	A	ug/L	2.05652	2.05652		2	0	0	0.0283	0.1	10	103%	80	120	0%	
Benzo(a)anthracene	A	ug/L	1.79001	1.79001		2	0	0	0.0272	0.1	10	90%	80	120	0%	
Benzo(a)pyrene	A	ug/L	1.86508	1.86508		2	0	0	0.0347	0.1	10	93%	80	120	0%	
Benzo(b)fluoranthene	A	ug/L	1.61026	1.61026		2	0	0	0.0226	0.1	10	81%	80	120	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14974167	10-Jan-22_CCV	SVOC-8270C-SI	CCV	√5975.I\sh0110221/10/2022	11:43:	1	R372987		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Benzo(g,h,i)perylene	A	ug/L	1.73901	1.73901		2	0	0	0.0267	0.1	10	87%	80	120	0%	
Benzo(k)fluoranthene	A	ug/L	1.84586	1.84586		2	0	0	0.0295	0.1	10	92%	80	120	0%	
Chrysene	A	ug/L	1.95655	1.95655		2	0	0	0.0458	0.1	10	98%	80	120	0%	
Dibenzo(a,h)anthracene	A	ug/L	1.7729	1.7729		2	0	0	0.0367	0.1	10	89%	80	120	0%	
Fluoranthene	A	ug/L	1.81637	1.81637		2	0	0	0.0233	0.1	10	91%	80	120	0%	
Fluorene	A	ug/L	1.90577	1.90577		2	0	0	0.0225	0.1	10	95%	80	120	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	1.6778	1.6778		2	0	0	0.0491	0.1	10	84%	80	120	0%	
Naphthalene	A	ug/L	1.90328	1.90328		2	0	0	0.029	0.1	10	95%	80	120	0%	
Phenanthrene	A	ug/L	1.89127	1.89127		2	0	0	0.0295	0.1	10	95%	80	120	0%	
Pyrene	A	ug/L	1.8362	1.8362		2	0	0	0.0239	0.1	10	92%	80	120	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1	10	0%	80	120	0%	
2-Fluorobiphenyl	S	ug/L	1.92679	1.92679		2	0	0	0.0444	0.1	10	96%	80	120	0%	
Nitrobenzene-d5	S	ug/L	1.70463	1.70463		2	0	0	0.0523	0.1	10	85%	80	120	0%	
Terphenyl-d14	S	ug/L	1.96182	1.96182		2	0	0	0.0563	0.1	10	98%	80	120	0%	
o-Terphenyl	X	ug/L	1.78408	1.78408		2	0	0	0.0654	0	0	89%	80	120	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14974168	10-Jan-22_ISTB	SVOC-8270C-SI	SAMP	√5975.I\sh0110221/10/2022	12:15:	1	R372987		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0206	0.1	10	0%	0	0	0%	
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0176	0.1	10	0%	0	0	0%	
Acenaphthene	A	ug/L	0	0		0	0	0	0.0317	0.1	10	0%	0	0	0%	
Acenaphthylene	A	ug/L	0	0		0	0	0	0.025	0.1	10	0%	0	0	0%	
Anthracene	A	ug/L	0	0		0	0	0	0.0283	0.1	10	0%	0	0	0%	
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.0272	0.1	10	0%	0	0	0%	
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.0347	0.1	10	0%	0	0	0%	
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.0226	0.1	10	0%	0	0	0%	
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.0267	0.1	10	0%	0	0	0%	
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.0295	0.1	10	0%	0	0	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14974168	10-Jan-22_ISTB	SVOC-8270C-SI SAMP		√5975.I\sh0110221/10/2022	12:15:	1	R372987		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Chrysene	A	ug/L	0	0		0	0	0	0.0458	0.1	10	0%	0	0	0%	
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.0367	0.1	10	0%	0	0	0%	
Fluoranthene	A	ug/L	0	0		0	0	0	0.0233	0.1	10	0%	0	0	0%	
Fluorene	A	ug/L	0	0		0	0	0	0.0225	0.1	10	0%	0	0	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.0491	0.1	10	0%	0	0	0%	
Naphthalene	A	ug/L	0	0		0	0	0	0.029	0.1	10	0%	0	0	0%	
Phenanthrene	A	ug/L	0	0		0	0	0	0.0295	0.1	10	0%	0	0	0%	
Pyrene	A	ug/L	0	0		0	0	0	0.0239	0.1	10	0%	0	0	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1	10	0%	0	0	0%	E
2-Fluorobiphenyl	S	ug/L	0	0		5	0	0	0.0444	0.1	10	0%	25	94	0%	S
Nitrobenzene-d5	S	ug/L	0	0		5	0	0	0.0523	0.1	10	0%	19	102	0%	S
Terphenyl-d14	S	ug/L	0	0		5	0	0	0.0563	0.1	10	0%	39	106	0%	S
o-Terphenyl	X	ug/L	0	0		200	0	0	0.0654	0	0	0%	40	140	0%	S

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14974169	MB-162577	SVOC-8270C-SI MBLK		√5975.I\sh0110221/10/2022	12:48:	1	162577	12/29/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0206	0.1	10	0%			0%	
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0176	0.1	10	0%			0%	
Acenaphthene	A	ug/L	0	0		0	0	0	0.0317	0.1	10	0%			0%	
Acenaphthylene	A	ug/L	0	0		0	0	0	0.025	0.1	10	0%			0%	
Anthracene	A	ug/L	0	0		0	0	0	0.0283	0.1	10	0%			0%	
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.0272	0.1	10	0%			0%	
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.0347	0.1	10	0%			0%	
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.0226	0.1	10	0%			0%	
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.0267	0.1	10	0%			0%	
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.0295	0.1	10	0%			0%	
Chrysene	A	ug/L	0	0		0	0	0	0.0458	0.1	10	0%			0%	
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.0367	0.1	10	0%			0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14974169	MB-162577	SVOC-8270C-SI MBLK		√5975.I\sh0110221	10/2022 12:48:	1	162577	12/29/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Fluoranthene	A	ug/L	0	0		0	0	0	0.0233	0.1	10	0%				0%
Fluorene	A	ug/L	0	0		0	0	0	0.0225	0.1	10	0%				0%
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.0491	0.1	10	0%				0%
Naphthalene	A	ug/L	0	0		0	0	0	0.029	0.1	10	0%				0%
Phenanthrene	A	ug/L	0	0		0	0	0	0.0295	0.1	10	0%				0%
Pyrene	A	ug/L	0	0		0	0	0	0.0239	0.1	10	0%				0%

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14974170	MB-162577	SVOC-8270C-SI MBLK		√5975.I\sh0110221	10/2022 1:20:2	20	162577	12/29/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14974171	LLCS-162577	SVOC-8270C-SI LCS-DOD		√5975.I\sh0110221	10/2022 1:53:0	1	162577	12/29/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	3.13854	3.13854		5	0	0	0.0206	0.1	10	63%	41	115		0%
2-Methylnaphthalene	A	ug/L	3.01302	3.01302		5	0	0	0.0176	0.1	10	60%	39	114		0%
Acenaphthene	A	ug/L	3.25251	3.25251		5	0	0	0.0317	0.1	10	65%	48	114		0%
Acenaphthylene	A	ug/L	3.4217	3.4217		5	0	0	0.025	0.1	10	68%	35	121		0%
Anthracene	A	ug/L	4.7558	4.7558		5	0	0	0.0283	0.1	10	95%	53	119		0%
Benzo(a)anthracene	A	ug/L	4.68426	4.68426		5	0	0	0.0272	0.1	10	94%	59	120		0%
Benzo(a)pyrene	A	ug/L	4.45456	4.45456		5	0	0	0.0347	0.1	10	89%	53	120		0%
Benzo(b)fluoranthene	A	ug/L	4.37384	4.37384		5	0	0	0.0226	0.1	10	87%	53	126		0%
Benzo(g,h,i)perylene	A	ug/L	4.63989	4.63989		5	0	0	0.0267	0.1	10	93%	44	128		0%
Benzo(k)fluoranthene	A	ug/L	4.30582	4.30582		5	0	0	0.0295	0.1	10	86%	54	125		0%
Chrysene	A	ug/L	4.82296	4.82296		5	0	0	0.0458	0.1	10	96%	57	120		0%
Dibenzo(a,h)anthracene	A	ug/L	4.71946	4.71946		5	0	0	0.0367	0.1	10	94%	44	141		0%
Fluoranthene	A	ug/L	4.48542	4.48542		5	0	0	0.0233	0.1	10	90%	58	120		0%
Fluorene	A	ug/L	4.03126	4.03126		5	0	0	0.0225	0.1	10	81%	50	118		0%
Indeno(1,2,3-cd)pyrene	A	ug/L	4.49394	4.49394		5	0	0	0.0491	0.1	10	90%	48	130		0%
Naphthalene	A	ug/L	2.84952	2.84952		5	0	0	0.029	0.1	10	57%	43	114		0%
Phenanthrene	A	ug/L	4.38645	4.38645		5	0	0	0.0295	0.1	10	88%	53	115		0%
Pyrene	A	ug/L	4.52121	4.52121		5	0	0	0.0239	0.1	10	90%	53	121		0%

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14974171	LLCS-162577	SVOC-8270C-SI	LCS-DOD	√5975.I\sh0110221	1/10/2022 1:53:0	1	162577	12/29/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
2-Fluorobiphenyl	S	ug/L	3.75008	3.75008		5	0	0	0.0444	0.1	10	75%	53	106	0%	
Nitrobenzene-d5	S	ug/L	3.45553	3.45553		5	0	0	0.0523	0.1	10	69%	55	111	0%	
Terphenyl-d14	S	ug/L	5.01046	5.01046		5	0	0	0.0563	0.1	10	100%	58	132	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14974172	LLCSD-162577	SVOC-8270C-SI	LCSD-DOD	√5975.I\sh0110221	1/10/2022 2:25:2	1	162577	12/29/2021	0	1E+07						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	2.92236	2.92236		5	0	3.13854	0.0206	0.1	10	58%	41	115	7%	
2-Methylnaphthalene	A	ug/L	2.84818	2.84818		5	0	3.01302	0.0176	0.1	10	57%	39	114	6%	
Acenaphthene	A	ug/L	3.13656	3.13656		5	0	3.25251	0.0317	0.1	10	63%	48	114	4%	
Acenaphthylene	A	ug/L	3.48274	3.48274		5	0	3.4217	0.025	0.1	10	70%	35	121	2%	
Anthracene	A	ug/L	4.89511	4.89511		5	0	4.7558	0.0283	0.1	10	98%	53	119	3%	
Benzo(a)anthracene	A	ug/L	4.9277	4.9277		5	0	4.68426	0.0272	0.1	10	99%	59	120	5%	
Benzo(a)pyrene	A	ug/L	4.56541	4.56541		5	0	4.45456	0.0347	0.1	10	91%	53	120	2%	
Benzo(b)fluoranthene	A	ug/L	4.5376	4.5376		5	0	4.37384	0.0226	0.1	10	91%	53	126	4%	
Benzo(g,h,i)perylene	A	ug/L	4.57493	4.57493		5	0	4.63989	0.0267	0.1	10	91%	44	128	1%	
Benzo(k)fluoranthene	A	ug/L	4.58327	4.58327		5	0	4.30582	0.0295	0.1	10	92%	54	125	6%	
Chrysene	A	ug/L	5.07999	5.07999		5	0	4.82296	0.0458	0.1	10	102%	57	120	5%	
Dibenzo(a,h)anthracene	A	ug/L	4.97475	4.97475		5	0	4.71946	0.0367	0.1	10	99%	44	141	5%	
Fluoranthene	A	ug/L	4.64944	4.64944		5	0	4.48542	0.0233	0.1	10	93%	58	120	4%	
Fluorene	A	ug/L	3.95441	3.95441		5	0	4.03126	0.0225	0.1	10	79%	50	118	2%	
Indeno(1,2,3-cd)pyrene	A	ug/L	4.72384	4.72384		5	0	4.49394	0.0491	0.1	10	94%	48	130	5%	
Naphthalene	A	ug/L	2.43305	2.43305		5	0	2.84952	0.029	0.1	10	49%	43	114	16%	
Phenanthrene	A	ug/L	4.59295	4.59295		5	0	4.38645	0.0295	0.1	10	92%	53	115	5%	
Pyrene	A	ug/L	4.78975	4.78975		5	0	4.52121	0.0239	0.1	10	96%	53	121	6%	
2-Fluorobiphenyl	S	ug/L	3.72519	3.72519		5	0	0	0.0444	0.1	10	75%	53	106	0%	
Nitrobenzene-d5	S	ug/L	3.7783	3.7783		5	0	0	0.0523	0.1	10	76%	55	111	0%	
Terphenyl-d14	S	ug/L	5.27057	5.27057		5	0	0	0.0563	0.1	10	105%	58	132	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14974173	B21122077-001	SVOC-8270C-SI	SAMP	√5975.I\sh0110221	1/10/2022 2:57:5	1	162577	12/29/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14974173	B21122077-001	SVOC-8270C-SI SAMP		√5975.I\sh0110221/10/2022	2:57:5	1	162577	12/29/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.020188	0.1	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.017248	0.1	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.031066	0.1	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.0245	0.1	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.027734	0.1	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.026656	0.1	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.034006	0.1	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.022148	0.1	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.026166	0.1	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.02891	0.1	10	0%	0	0	0%	U
Chrysene	A	ug/L	0	0		0	0	0	0.044884	0.1	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.035966	0.1	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0	0		0	0	0	0.022834	0.1	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.02205	0.1	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.048118	0.1	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.02842	0.1	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.02891	0.1	10	0%	0	0	0%	U
Pyrene	A	ug/L	0	0		0	0	0	0.023422	0.1	10	0%	0	0	0%	U

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14974174	B21122077-001	SVOC-8270C-SI SAMP		√5975.I\sh0110221/10/2022	3:30:1	20	162577	12/29/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14974175	B21122088-001	SVOC-8270C-SI SAMP		√5975.I\sh0110221/10/2022	4:02:4	1	162577	12/29/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.02163	0.105	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.01848	0.105	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.033285	0.105	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.02625	0.105	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.029715	0.105	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.02856	0.105	10	0%	0	0	0%	U

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14974175	B21122088-001	SVOC-8270C-SI SAMP		√5975.I\sh0110221/10/2022	4:02:4	1	162577	12/29/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.036435	0.105	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.02373	0.105	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.028035	0.105	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.030975	0.105	10	0%	0	0	0%	U
Chrysene	A	ug/L	0	0		0	0	0	0.04809	0.105	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.038535	0.105	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0	0		0	0	0	0.024465	0.105	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.023625	0.105	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.051555	0.105	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.03045	0.105	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.030975	0.105	10	0%	0	0	0%	U
Pyrene	A	ug/L	0	0		0	0	0	0.025095	0.105	10	0%	0	0	0%	U

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14974176	B21122088-001	SVOC-8270C-SI SAMP		√5975.I\sh0110221/10/2022	4:35:0	20	162577	12/29/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14974177	B21122090-001	SVOC-8270C-SI SAMP		√5975.I\sh0110221/10/2022	5:07:2	1	162577	12/29/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0206	0.1	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0176	0.1	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.0317	0.1	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.025	0.1	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.0283	0.1	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.0272	0.1	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.0347	0.1	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.0226	0.1	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.0267	0.1	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.0295	0.1	10	0%	0	0	0%	U
Chrysene	A	ug/L	0	0		0	0	0	0.0458	0.1	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.0367	0.1	10	0%	0	0	0%	U

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14974177	B21122090-001	SVOC-8270C-SI SAMP		√5975.I\sh0110221	10/2022 5:07:2	1	162577	12/29/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Fluoranthene	A	ug/L	0	0		0	0	0	0.0233	0.1	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.0225	0.1	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.0491	0.1	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.029	0.1	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.0295	0.1	10	0%	0	0	0%	U
Pyrene	A	ug/L	0	0		0	0	0	0.0239	0.1	10	0%	0	0	0%	U

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14974178	B21122090-001	SVOC-8270C-SI SAMP		√5975.I\sh0110221	10/2022 5:39:4	20	162577	12/29/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14974179	B21122105-001	SVOC-8270C-SI SAMP		√5975.I\sh0110221	10/2022 6:12:0	1	162577	12/29/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0198172	0.1	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0169312	0.1	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.0304954	0.1	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.02405	0.1	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.0272246	0.1	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.0261664	0.1	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.0333814	0.1	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.0217412	0.1	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.0256854	0.1	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.028379	0.1	10	0%	0	0	0%	U
Chrysene	A	ug/L	0	0		0	0	0	0.0440596	0.1	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.0353054	0.1	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0	0		0	0	0	0.0224146	0.1	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.021645	0.1	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.0472342	0.1	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.027898	0.1	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.028379	0.1	10	0%	0	0	0%	U
Pyrene	A	ug/L	0	0		0	0	0	0.0229918	0.1	10	0%	0	0	0%	U

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14974180	B21122105-001	SVOC-8270C-SI SAMP		√5975.I\sh0110221	10/2022 6:44:2	20	162577	12/29/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14974181	B21122105-001	SVOC-8270C-SI MS-DOD		√5975.I\sh0110221	10/2022 7:16:5	1	162577	12/29/2021	1E+07	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	3.78436	3.78436		5	0	0	0.0206	0.1	10	76%	41	115	0%	
2-Methylnaphthalene	A	ug/L	3.60519	3.60519		5	0	0	0.0176	0.1	10	72%	39	114	0%	
Acenaphthene	A	ug/L	3.74233	3.74233		5	0	0	0.0317	0.1	10	75%	48	114	0%	
Acenaphthylene	A	ug/L	3.97721	3.97721		5	0	0	0.025	0.1	10	80%	35	121	0%	
Anthracene	A	ug/L	4.98635	4.98635		5	0	0	0.0283	0.1	10	100%	53	119	0%	
Benzo(a)anthracene	A	ug/L	5.01224	5.01224		5	0	0	0.0272	0.1	10	100%	59	120	0%	
Benzo(a)pyrene	A	ug/L	4.39522	4.39522		5	0	0	0.0347	0.1	10	88%	53	120	0%	
Benzo(b)fluoranthene	A	ug/L	4.40542	4.40542		5	0	0	0.0226	0.1	10	88%	53	126	0%	
Benzo(g,h,i)perylene	A	ug/L	4.6213	4.6213		5	0	0	0.0267	0.1	10	92%	44	128	0%	
Benzo(k)fluoranthene	A	ug/L	4.49059	4.49059		5	0	0	0.0295	0.1	10	90%	54	125	0%	
Chrysene	A	ug/L	5.04118	5.04118		5	0	0	0.0458	0.1	10	101%	57	120	0%	
Dibenzo(a,h)anthracene	A	ug/L	4.69611	4.69611		5	0	0	0.0367	0.1	10	94%	44	141	0%	
Fluoranthene	A	ug/L	4.6696	4.6696		5	0	0	0.0233	0.1	10	93%	58	120	0%	
Fluorene	A	ug/L	4.5106	4.5106		5	0	0	0.0225	0.1	10	90%	50	118	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	4.29735	4.29735		5	0	0	0.0491	0.1	10	86%	48	130	0%	
Naphthalene	A	ug/L	3.28255	3.28255		5	0	0	0.029	0.1	10	66%	43	114	0%	
Phenanthrene	A	ug/L	4.73202	4.73202		5	0	0	0.0295	0.1	10	95%	53	115	0%	
Pyrene	A	ug/L	4.65673	4.65673		5	0	0	0.0239	0.1	10	93%	53	121	0%	
2-Fluorobiphenyl	S	ug/L	3.941	3.941		5	0	0	0.0444	0.1	10	79%	53	106	0%	
Nitrobenzene-d5	S	ug/L	3.09846	3.09846		5	0	0	0.0523	0.1	10	62%	55	111	0%	
Terphenyl-d14	S	ug/L	5.11748	5.11748		5	0	0	0.0563	0.1	10	102%	58	132	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14974182	MB-162701	SVOC-8270C-SI MBLK		√5975.I\sh0110221	10/2022 7:49:1	1	162701	1/4/2022 3:4	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0206	0.1	10	0%			0%	
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0176	0.1	10	0%			0%	
Acenaphthene	A	ug/L	0	0		0	0	0	0.0317	0.1	10	0%			0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14974182	MB-162701	SVOC-8270C-SI	MBLK	√5975.I\sh0110221	10/2022 7:49:1	1	162701	1/4/2022 3:4	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Acenaphthylene	A	ug/L	0	0		0	0	0	0.025	0.1	10	0%			0%	
Anthracene	A	ug/L	0	0		0	0	0	0.0283	0.1	10	0%			0%	
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.0272	0.1	10	0%			0%	
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.0347	0.1	10	0%			0%	
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.0226	0.1	10	0%			0%	
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.0267	0.1	10	0%			0%	
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.0295	0.1	10	0%			0%	
Chrysene	A	ug/L	0	0		0	0	0	0.0458	0.1	10	0%			0%	
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.0367	0.1	10	0%			0%	
Fluoranthene	A	ug/L	0	0		0	0	0	0.0233	0.1	10	0%			0%	
Fluorene	A	ug/L	0	0		0	0	0	0.0225	0.1	10	0%			0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.0491	0.1	10	0%			0%	
Naphthalene	A	ug/L	0	0		0	0	0	0.029	0.1	10	0%			0%	
Phenanthrene	A	ug/L	0	0		0	0	0	0.0295	0.1	10	0%			0%	
Pyrene	A	ug/L	0	0		0	0	0	0.0239	0.1	10	0%			0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14974183	MB-162701	SVOC-8270C-SI	MBLK	√5975.I\sh0110221	10/2022 8:21:3	20	162701	1/4/2022 3:4	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14974184	LLCS-162701	SVOC-8270C-SI	LCS-DOD	√5975.I\sh0110221	10/2022 8:53:5	1	162701	1/4/2022 3:4	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	3.82578	3.82578		5	0	0	0.0206	0.1	10	77%	41	115	0%	
2-Methylnaphthalene	A	ug/L	3.61943	3.61943		5	0	0	0.0176	0.1	10	72%	39	114	0%	
Acenaphthene	A	ug/L	3.55205	3.55205		5	0	0	0.0317	0.1	10	71%	48	114	0%	
Acenaphthylene	A	ug/L	3.77187	3.77187		5	0	0	0.025	0.1	10	75%	35	121	0%	
Anthracene	A	ug/L	4.47355	4.47355		5	0	0	0.0283	0.1	10	89%	53	119	0%	
Benzo(a)anthracene	A	ug/L	4.38375	4.38375		5	0	0	0.0272	0.1	10	88%	59	120	0%	
Benzo(a)pyrene	A	ug/L	4.00927	4.00927		5	0	0	0.0347	0.1	10	80%	53	120	0%	
Benzo(b)fluoranthene	A	ug/L	4.03231	4.03231		5	0	0	0.0226	0.1	10	81%	53	126	0%	
Benzo(g,h,i)perylene	A	ug/L	4.24138	4.24138		5	0	0	0.0267	0.1	10	85%	44	128	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14974184	LLCS-162701	SVOC-8270C-SI	LCS-DOD	√5975.I\sh0110221	10/2022 8:53:5	1	162701	1/4/2022 3:4	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Benzo(k)fluoranthene	A	ug/L	4.16296	4.16296		5	0	0	0.0295	0.1	10	83%	54	125	0%	
Chrysene	A	ug/L	4.48354	4.48354		5	0	0	0.0458	0.1	10	90%	57	120	0%	
Dibenzo(a,h)anthracene	A	ug/L	4.18259	4.18259		5	0	0	0.0367	0.1	10	84%	44	141	0%	
Fluoranthene	A	ug/L	4.02741	4.02741		5	0	0	0.0233	0.1	10	81%	58	120	0%	
Fluorene	A	ug/L	4.06961	4.06961		5	0	0	0.0225	0.1	10	81%	50	118	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	4.01732	4.01732		5	0	0	0.0491	0.1	10	80%	48	130	0%	
Naphthalene	A	ug/L	3.44371	3.44371		5	0	0	0.029	0.1	10	69%	43	114	0%	
Phenanthrene	A	ug/L	4.20217	4.20217		5	0	0	0.0295	0.1	10	84%	53	115	0%	
Pyrene	A	ug/L	4.02576	4.02576		5	0	0	0.0239	0.1	10	81%	53	121	0%	
2-Fluorobiphenyl	S	ug/L	3.74398	3.74398		5	0	0	0.0444	0.1	10	75%	53	106	0%	
Nitrobenzene-d5	S	ug/L	3.40025	3.40025		5	0	0	0.0523	0.1	10	68%	55	111	0%	
Terphenyl-d14	S	ug/L	4.60733	4.60733		5	0	0	0.0563	0.1	10	92%	58	132	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14974185	LLCSD-162701	SVOC-8270C-SI	LLCSD-DOD	√5975.I\sh0110221	10/2022 9:26:2	1	162701	1/4/2022 3:4	0	1E+07						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	3.88411	3.88411		5	0	3.82578	0.0206	0.1	10	78%	41	115	2%	
2-Methylnaphthalene	A	ug/L	3.69507	3.69507		5	0	3.61943	0.0176	0.1	10	74%	39	114	2%	
Acenaphthene	A	ug/L	3.79029	3.79029		5	0	3.55205	0.0317	0.1	10	76%	48	114	6%	
Acenaphthylene	A	ug/L	3.96129	3.96129		5	0	3.77187	0.025	0.1	10	79%	35	121	5%	
Anthracene	A	ug/L	4.54194	4.54194		5	0	4.47355	0.0283	0.1	10	91%	53	119	2%	
Benzo(a)anthracene	A	ug/L	4.4757	4.4757		5	0	4.38375	0.0272	0.1	10	90%	59	120	2%	
Benzo(a)pyrene	A	ug/L	3.98387	3.98387		5	0	4.00927	0.0347	0.1	10	80%	53	120	1%	
Benzo(b)fluoranthene	A	ug/L	3.93104	3.93104		5	0	4.03231	0.0226	0.1	10	79%	53	126	3%	
Benzo(g,h,i)perylene	A	ug/L	4.15901	4.15901		5	0	4.24138	0.0267	0.1	10	83%	44	128	2%	
Benzo(k)fluoranthene	A	ug/L	4.04506	4.04506		5	0	4.16296	0.0295	0.1	10	81%	54	125	3%	
Chrysene	A	ug/L	4.47689	4.47689		5	0	4.48354	0.0458	0.1	10	90%	57	120	0%	
Dibenzo(a,h)anthracene	A	ug/L	4.24952	4.24952		5	0	4.18259	0.0367	0.1	10	85%	44	141	2%	
Fluoranthene	A	ug/L	4.24824	4.24824		5	0	4.02741	0.0233	0.1	10	85%	58	120	5%	
Fluorene	A	ug/L	4.14584	4.14584		5	0	4.06961	0.0225	0.1	10	83%	50	118	2%	
Indeno(1,2,3-cd)pyrene	A	ug/L	4.03105	4.03105		5	0	4.01732	0.0491	0.1	10	81%	48	130	0%	
Naphthalene	A	ug/L	3.44292	3.44292		5	0	3.44371	0.029	0.1	10	69%	43	114	0%	
Phenanthrene	A	ug/L	4.23911	4.23911		5	0	4.20217	0.0295	0.1	10	85%	53	115	1%	
Pyrene	A	ug/L	4.12444	4.12444		5	0	4.02576	0.0239	0.1	10	82%	53	121	2%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14974185	LLCSD-162701	SVOC-8270C-SI	LCSD-DOD	√5975.I\sh0110221	1/10/2022 9:26:2	1	162701	1/4/2022 3:4	0	1E+07						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
2-Fluorobiphenyl	S	ug/L	3.80294	3.80294		5	0	0	0.0444	0.1	10	76%	53	106	0%	
Nitrobenzene-d5	S	ug/L	3.02278	3.02278		5	0	0	0.0523	0.1	10	60%	55	111	0%	
Terphenyl-d14	S	ug/L	4.71004	4.71004		5	0	0	0.0563	0.1	10	94%	58	132	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14974186	B22010096-001	SVOC-8270C-SI	SAMP	√5975.I\sh0110221	1/10/2022 9:58:3	1	162701	1/4/2022 3:4	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.020188	0.1	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.017248	0.1	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.031066	0.1	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.0245	0.1	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.027734	0.1	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.026656	0.1	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.034006	0.1	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.022148	0.1	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.026166	0.1	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.02891	0.1	10	0%	0	0	0%	U
Chrysene	A	ug/L	0	0		0	0	0	0.044884	0.1	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.035966	0.1	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0	0		0	0	0	0.022834	0.1	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.02205	0.1	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.048118	0.1	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.02842	0.1	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.02891	0.1	10	0%	0	0	0%	U
Pyrene	A	ug/L	0	0		0	0	0	0.023422	0.1	10	0%	0	0	0%	U

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14974187	B22010096-001	SVOC-8270C-SI	SAMP	√5975.I\sh0110221	1/10/2022 10:31:	20	162701	1/4/2022 3:4	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14974188	10-Jan-22_CCV	SVOC-8270C-SI	CCV	√5975.I\sh0110221	10/2022 11:03:	1	R372987		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	2.22886	2.22886		2	0	0	0.0206	0.1	10	111%	80	120	0%	
2-Methylnaphthalene	A	ug/L	1.96397	1.96397		2	0	0	0.0176	0.1	10	98%	80	120	0%	
Acenaphthene	A	ug/L	1.63173	1.63173		2	0	0	0.0317	0.1	10	82%	80	120	0%	
Acenaphthylene	A	ug/L	1.80571	1.80571		2	0	0	0.025	0.1	10	90%	80	120	0%	
Anthracene	A	ug/L	1.97567	1.97567		2	0	0	0.0283	0.1	10	99%	80	120	0%	
Benzo(a)anthracene	A	ug/L	1.88359	1.88359		2	0	0	0.0272	0.1	10	94%	80	120	0%	
Benzo(a)pyrene	A	ug/L	1.81243	1.81243		2	0	0	0.0347	0.1	10	91%	80	120	0%	
Benzo(b)fluoranthene	A	ug/L	1.63805	1.63805		2	0	0	0.0226	0.1	10	82%	80	120	0%	
Benzo(g,h,i)perylene	A	ug/L	1.80772	1.80772		2	0	0	0.0267	0.1	10	90%	80	120	0%	
Benzo(k)fluoranthene	A	ug/L	1.84679	1.84679		2	0	0	0.0295	0.1	10	92%	80	120	0%	
Chrysene	A	ug/L	1.93334	1.93334		2	0	0	0.0458	0.1	10	97%	80	120	0%	
Dibenzo(a,h)anthracene	A	ug/L	1.75907	1.75907		2	0	0	0.0367	0.1	10	88%	80	120	0%	
Fluoranthene	A	ug/L	1.82612	1.82612		2	0	0	0.0233	0.1	10	91%	80	120	0%	
Fluorene	A	ug/L	1.91688	1.91688		2	0	0	0.0225	0.1	10	96%	80	120	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	1.65867	1.65867		2	0	0	0.0491	0.1	10	83%	80	120	0%	
Naphthalene	A	ug/L	1.86331	1.86331		2	0	0	0.029	0.1	10	93%	80	120	0%	
Phenanthrene	A	ug/L	1.93848	1.93848		2	0	0	0.0295	0.1	10	97%	80	120	0%	
Pyrene	A	ug/L	1.78881	1.78881		2	0	0	0.0239	0.1	10	89%	80	120	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1	10	0%	80	120	0%	
2-Fluorobiphenyl	S	ug/L	1.87756	1.87756		2	0	0	0.0444	0.1	10	94%	80	120	0%	
Nitrobenzene-d5	S	ug/L	1.68113	1.68113		2	0	0	0.0523	0.1	10	84%	80	120	0%	
Terphenyl-d14	S	ug/L	1.99684	1.99684		2	0	0	0.0563	0.1	10	100%	80	120	0%	
o-Terphenyl	X	ug/L	1.73962	1.73962		2	0	0	0.0654	0	0	87%	80	120	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15044394	LLCS-162577	SVOC-8270-W-	LCS	√5975.I\sh0110221	10/2022 1:53:0	1	162577	12/29/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15044394	LLCS-162577	SVOC-8270-W-	LCS	√5975.I\sh0110221	10/2022 1:53:0	1	162577	12/29/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	3.13854	3.13854		5	0	0	0.0206	0.1	10	63%	18	117	0%	
2-Methylnaphthalene	A	ug/L	3.01302	3.01302		5	0	0	0.0176	0.1	10	60%	18	117	0%	
Acenaphthene	A	ug/L	3.25251	3.25251		5	0	0	0.0317	0.1	10	65%	40	92	0%	
Acenaphthylene	A	ug/L	3.4217	3.4217		5	0	0	0.025	0.1	10	68%	37	96	0%	
Anthracene	A	ug/L	4.7558	4.7558		5	0	0	0.0283	0.1	10	95%	46	108	0%	
Benzo(a)anthracene	A	ug/L	4.68426	4.68426		5	0	0	0.0272	0.1	10	94%	41	105	0%	
Benzo(a)pyrene	A	ug/L	4.45456	4.45456		5	0	0	0.0347	0.1	10	89%	42	110	0%	
Benzo(b)fluoranthene	A	ug/L	4.37384	4.37384		5	0	0	0.0226	0.1	10	87%	27	121	0%	
Benzo(g,h,i)perylene	A	ug/L	4.63989	4.63989		5	0	0	0.0267	0.1	10	93%	44	108	0%	
Benzo(k)fluoranthene	A	ug/L	4.30582	4.30582		5	0	0	0.0295	0.1	10	86%	44	111	0%	
Chrysene	A	ug/L	4.82296	4.82296		5	0	0	0.0458	0.1	10	96%	50	106	0%	
Dibenzo(a,h)anthracene	A	ug/L	4.71946	4.71946		5	0	0	0.0367	0.1	10	94%	47	111	0%	
Fluoranthene	A	ug/L	4.48542	4.48542		5	0	0	0.0233	0.1	10	90%	44	111	0%	
Fluorene	A	ug/L	4.03126	4.03126		5	0	0	0.0225	0.1	10	81%	42	99	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	4.49394	4.49394		5	0	0	0.0491	0.1	10	90%	33	112	0%	
Naphthalene	A	ug/L	2.84952	2.84952		5	0	0	0.029	0.1	10	57%	22	108	0%	
Phenanthrene	A	ug/L	4.38645	4.38645		5	0	0	0.0295	0.1	10	88%	43	106	0%	
Pyrene	A	ug/L	4.52121	4.52121		5	0	0	0.0239	0.1	10	90%	41	106	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
2-Fluorobiphenyl	S	ug/L	3.75008	3.75008		5	0	0	0.0444	0.1	10	75%	25	94	0%	
Nitrobenzene-d5	S	ug/L	3.45553	3.45553		5	0	0	0.0523	0.1	10	69%	19	102	0%	
Terphenyl-d14	S	ug/L	5.01046	5.01046		5	0	0	0.0563	0.1	10	100%	39	106	0%	
o-Terphenyl	X	ug/L	4.08365	4.08365		5	0	0	0.0654	0.1	10	82%	40	140	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15044396	LLCSD-162577	SVOC-8270-W-	LLCSD	√5975.I\sh0110221	10/2022 2:25:2	1	162577	12/29/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15044396	LLCSD-162577	SVOC-8270-W-	LCSD	√5975.I\sh0110221/10/2022	2:25:2	1	162577	12/29/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	2.92236	2.92236		5	0	0	0.0206	0.1	10	58%	18	117	0%	
2-Methylnaphthalene	A	ug/L	2.84818	2.84818		5	0	0	0.0176	0.1	10	57%	18	117	0%	
Acenaphthene	A	ug/L	3.13656	3.13656		5	0	0	0.0317	0.1	10	63%	40	92	0%	
Acenaphthylene	A	ug/L	3.48274	3.48274		5	0	0	0.025	0.1	10	70%	37	96	0%	
Anthracene	A	ug/L	4.89511	4.89511		5	0	0	0.0283	0.1	10	98%	46	108	0%	
Benzo(a)anthracene	A	ug/L	4.9277	4.9277		5	0	0	0.0272	0.1	10	99%	41	105	0%	
Benzo(a)pyrene	A	ug/L	4.56541	4.56541		5	0	0	0.0347	0.1	10	91%	42	110	0%	
Benzo(b)fluoranthene	A	ug/L	4.5376	4.5376		5	0	0	0.0226	0.1	10	91%	27	121	0%	
Benzo(g,h,i)perylene	A	ug/L	4.57493	4.57493		5	0	0	0.0267	0.1	10	91%	44	108	0%	
Benzo(k)fluoranthene	A	ug/L	4.58327	4.58327		5	0	0	0.0295	0.1	10	92%	44	111	0%	
Chrysene	A	ug/L	5.07999	5.07999		5	0	0	0.0458	0.1	10	102%	50	106	0%	
Dibenzo(a,h)anthracene	A	ug/L	4.97475	4.97475		5	0	0	0.0367	0.1	10	99%	47	111	0%	
Fluoranthene	A	ug/L	4.64944	4.64944		5	0	0	0.0233	0.1	10	93%	44	111	0%	
Fluorene	A	ug/L	3.95441	3.95441		5	0	0	0.0225	0.1	10	79%	42	99	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	4.72384	4.72384		5	0	0	0.0491	0.1	10	94%	33	112	0%	
Naphthalene	A	ug/L	2.43305	2.43305		5	0	0	0.029	0.1	10	49%	22	108	0%	
Phenanthrene	A	ug/L	4.59295	4.59295		5	0	0	0.0295	0.1	10	92%	43	106	0%	
Pyrene	A	ug/L	4.78975	4.78975		5	0	0	0.0239	0.1	10	96%	41	106	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
2-Fluorobiphenyl	S	ug/L	3.72519	3.72519		5	0	0	0.0444	0.1	10	75%	25	94	0%	
Nitrobenzene-d5	S	ug/L	3.7783	3.7783		5	0	0	0.0523	0.1	10	76%	19	102	0%	
Terphenyl-d14	S	ug/L	5.27057	5.27057		5	0	0	0.0563	0.1	10	105%	39	106	0%	
o-Terphenyl	X	ug/L	4.33768	4.33768		5	0	0	0.0654	0.1	10	87%	40	140	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15044397	LLCS-162701	SVOC-8270-W-	LCS	√5975.I\sh0110221/10/2022	8:53:5	1	162701	1/4/2022	3:4	0	0					
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15044397	LLCS-162701	SVOC-8270-W-	LCS	√5975.I\sh0110221	10/2022 8:53:5	1	162701	1/4/2022 3:4	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	3.82578	3.82578		5	0	0	0.0206	0.1	10	77%	18	117	0%	
2-Methylnaphthalene	A	ug/L	3.61943	3.61943		5	0	0	0.0176	0.1	10	72%	18	117	0%	
Acenaphthene	A	ug/L	3.55205	3.55205		5	0	0	0.0317	0.1	10	71%	40	92	0%	
Acenaphthylene	A	ug/L	3.77187	3.77187		5	0	0	0.025	0.1	10	75%	37	96	0%	
Anthracene	A	ug/L	4.47355	4.47355		5	0	0	0.0283	0.1	10	89%	46	108	0%	
Benzo(a)anthracene	A	ug/L	4.38375	4.38375		5	0	0	0.0272	0.1	10	88%	41	105	0%	
Benzo(a)pyrene	A	ug/L	4.00927	4.00927		5	0	0	0.0347	0.1	10	80%	42	110	0%	
Benzo(b)fluoranthene	A	ug/L	4.03231	4.03231		5	0	0	0.0226	0.1	10	81%	27	121	0%	
Benzo(g,h,i)perylene	A	ug/L	4.24138	4.24138		5	0	0	0.0267	0.1	10	85%	44	108	0%	
Benzo(k)fluoranthene	A	ug/L	4.16296	4.16296		5	0	0	0.0295	0.1	10	83%	44	111	0%	
Chrysene	A	ug/L	4.48354	4.48354		5	0	0	0.0458	0.1	10	90%	50	106	0%	
Dibenzo(a,h)anthracene	A	ug/L	4.18259	4.18259		5	0	0	0.0367	0.1	10	84%	47	111	0%	
Fluoranthene	A	ug/L	4.02741	4.02741		5	0	0	0.0233	0.1	10	81%	44	111	0%	
Fluorene	A	ug/L	4.06961	4.06961		5	0	0	0.0225	0.1	10	81%	42	99	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	4.01732	4.01732		5	0	0	0.0491	0.1	10	80%	33	112	0%	
Naphthalene	A	ug/L	3.44371	3.44371		5	0	0	0.029	0.1	10	69%	22	108	0%	
Phenanthrene	A	ug/L	4.20217	4.20217		5	0	0	0.0295	0.1	10	84%	43	106	0%	
Pyrene	A	ug/L	4.02576	4.02576		5	0	0	0.0239	0.1	10	81%	41	106	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
2-Fluorobiphenyl	S	ug/L	3.74398	3.74398		5	0	0	0.0444	0.1	10	75%	25	94	0%	
Nitrobenzene-d5	S	ug/L	3.40025	3.40025		5	0	0	0.0523	0.1	10	68%	19	102	0%	
Terphenyl-d14	S	ug/L	4.60733	4.60733		5	0	0	0.0563	0.1	10	92%	39	106	0%	
o-Terphenyl	X	ug/L	3.85555	3.85555		5	0	0	0.0654	0.1	10	77%	40	140	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15044399	LLCSD-162701	SVOC-8270-W-	LLCSD	√5975.I\sh0110221	10/2022 9:26:2	1	162701	1/4/2022 3:4	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15044399	LLCSD-162701	SVOC-8270-W-	LCSD	√5975.I\sh0110221	10/2022 9:26:2	1	162701	1/4/2022 3:4	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	3.88411	3.88411		5	0	0	0.0206	0.1	10	78%	18	117	0%	
2-Methylnaphthalene	A	ug/L	3.69507	3.69507		5	0	0	0.0176	0.1	10	74%	18	117	0%	
Acenaphthene	A	ug/L	3.79029	3.79029		5	0	0	0.0317	0.1	10	76%	40	92	0%	
Acenaphthylene	A	ug/L	3.96129	3.96129		5	0	0	0.025	0.1	10	79%	37	96	0%	
Anthracene	A	ug/L	4.54194	4.54194		5	0	0	0.0283	0.1	10	91%	46	108	0%	
Benzo(a)anthracene	A	ug/L	4.4757	4.4757		5	0	0	0.0272	0.1	10	90%	41	105	0%	
Benzo(a)pyrene	A	ug/L	3.98387	3.98387		5	0	0	0.0347	0.1	10	80%	42	110	0%	
Benzo(b)fluoranthene	A	ug/L	3.93104	3.93104		5	0	0	0.0226	0.1	10	79%	27	121	0%	
Benzo(g,h,i)perylene	A	ug/L	4.15901	4.15901		5	0	0	0.0267	0.1	10	83%	44	108	0%	
Benzo(k)fluoranthene	A	ug/L	4.04506	4.04506		5	0	0	0.0295	0.1	10	81%	44	111	0%	
Chrysene	A	ug/L	4.47689	4.47689		5	0	0	0.0458	0.1	10	90%	50	106	0%	
Dibenzo(a,h)anthracene	A	ug/L	4.24952	4.24952		5	0	0	0.0367	0.1	10	85%	47	111	0%	
Fluoranthene	A	ug/L	4.24824	4.24824		5	0	0	0.0233	0.1	10	85%	44	111	0%	
Fluorene	A	ug/L	4.14584	4.14584		5	0	0	0.0225	0.1	10	83%	42	99	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	4.03105	4.03105		5	0	0	0.0491	0.1	10	81%	33	112	0%	
Naphthalene	A	ug/L	3.44292	3.44292		5	0	0	0.029	0.1	10	69%	22	108	0%	
Phenanthrene	A	ug/L	4.23911	4.23911		5	0	0	0.0295	0.1	10	85%	43	106	0%	
Pyrene	A	ug/L	4.12444	4.12444		5	0	0	0.0239	0.1	10	82%	41	106	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
2-Fluorobiphenyl	S	ug/L	3.80294	3.80294		5	0	0	0.0444	0.1	10	76%	25	94	0%	
Nitrobenzene-d5	S	ug/L	3.02278	3.02278		5	0	0	0.0523	0.1	10	60%	19	102	0%	
Terphenyl-d14	S	ug/L	4.71004	4.71004		5	0	0	0.0563	0.1	10	94%	39	106	0%	
o-Terphenyl	X	ug/L	3.90641	3.90641		5	0	0	0.0654	0.1	10	78%	40	140	0%	



Write Sequence

Insert Entries(Have the first cell for entries selecte)

File Name	Sample Name	Line No.	Test Code	Multiplier	Divisor	Method Name
Jan1001.d	10-Jan-22_TUNE_1	1		1	1	5975Tune.M
Jan1002.d	10-Jan-22_CCV_2	2	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1003.d	10-Jan-22_ISTBLK_3	3	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1004.d	MB-162577	4	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1005.d	MB-162577	5	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Jan1006.d	LLCS-162577	6	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1007.d	LLCSD-162577	7	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1008.d	B21122077-001C	8	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1009.d	B21122077-001C	9	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Jan1010.d	B21122088-001C	10	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1011.d	B21122088-001C	11	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Jan1012.d	B21122090-001C	12	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1013.d	B21122090-001C	13	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Jan1014.d	B21122105-001C	14	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1015.d	B21122105-001C	15	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Jan1016.d	B21122105-001CLMS	16	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1017.d	MB-162701	17	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1018.d	MB-162701	18	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Jan1019.d	LLCS-162701	19	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1020.d	LLCSD-162701	20	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1021.d	B22010096-001C	21	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1022.d	B22010096-001C	22	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Jan1023.d	10-Jan-22_CCV_23	23	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1024.d	10-Jan-22_TUNE_24	24		1	1	5975Tune.M
Jan1025.d	10-Jan-22_CCV_25	25	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1026.d	10-Jan-22_ISTBLK_26	26	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1027.d	B22010120-001C	27	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1028.d	B22010120-001C	28	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Jan1029.d	B22010134-001C	29	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1030.d	B22010134-001C	30	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Jan1031.d	B22010141-001C	31	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1032.d	B22010141-001C	32	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Jan1033.d	B22010141-001CLMS	33	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1034.d	B22010142-001C	34	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1035.d	B22010142-001C	35	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Jan1036.d	B22010143-001C	36	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1037.d	B22010143-001C	37	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Jan1038.d	B22010145-001C	38	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1039.d	B22010145-001C	39	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Jan1040.d	B22010148-001C	40	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1041.d	B22010148-001C	41	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Jan1042.d	B22010209-001C	42	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1043.d	B22010209-001C	43	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Jan1044.d	B22010211-001C	44	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1045.d	B22010211-001C	45	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Jan1046.d	10-Jan-22_CCV_46	46	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1047.d	11-Jan-22_TUNE_47	47		1	1	5975Tune.M
Jan1048.d	11-Jan-22_CCV_48	48	SVOC-8270-S-LLPAH	1	1	5975BNASIM.M
Jan1049.d	11-Jan-22_ISTBLK_49	49	SVOC-8270-S-LLPAH	1	1	5975BNASIM.M
Jan1050.d	MB-162835-59687-59601	50	SVOC-8270-S-LLPAH	1	1	5975BNASIM.M
Jan1051.d	MB-162835-59687-59601	51	SVOC-8270-S-LLPAH	20	1	5975BNASIM.M
Jan1052.d	LCS-162835-59687-59601	52	SVOC-8270-S-LLPAH	20	1	5975BNASIM.M
Jan1053.d	H21120525-005A	53	SVOC-8270-S-LLPAH	20	1	5975BNASIM.M
Jan1054.d	H21120525-005AMS	54	SVOC-8270-S-LLPAH	20	1	5975BNASIM.M
Jan1055.d	H21120525-005AMSD	55	SVOC-8270-S-LLPAH	20	1	5975BNASIM.M
Jan1056.d	B21121830-001A	56	SVOC-8270-S-LLPAH	1	1	5975BNASIM.M
Jan1057.d	B21121830-001A	57	SVOC-8270-S-LLPAH	20	1	5975BNASIM.M
Jan1058.d	B21121830-002A	58	SVOC-8270-S-LLPAH	1	1	5975BNASIM.M
Jan1059.d	B21121830-002A	59	SVOC-8270-S-LLPAH	20	1	5975BNASIM.M









Tune Evaluation Report

Data Path: \\MASSHUNTER\Org\Data\SV5975.I\sh011022\1 e8270d bna SIM\Jan1001.D
 Acq on: 1/10/2022 11:19:40 AM
 Operator: LIMS import
 Sample: 10-Jan-22_TUNE_1
 Inst Name: GCMS
 ALS Vial: 1
 Method: \\MASSHUNTER\Org\Data\SV5975.I\Methods\DFTPP5975625.m




Target Mass	Rel. To Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Pass/Fail
51	198	30	60	46.9	143808	Pass
68	69	0	2	0.0	0	Pass
70	69	0	2	0.5	1124	Pass
127	198	40	60	52.8	161856	Pass
197	198	0	1	0.0	0	Pass
198	198	100	100	100.0	306560	Pass
199	198	5	9	7.1	21696	Pass
275	198	10	30	29.5	90576	Pass
365	198	1	100	3.7	11409	Pass
441	443	1E-10	150	89.9	42704	Pass
442	198	40	100	80.7	247360	Pass
443	442	17	23	19.2	47528	Pass
69	69	100	100	100.0	227904	Pass

Tune Evaluation Report



Tune Evaluation Report


+ Scan (rt: 8.181-8.220 min, 28 scans) Jan1001.D 4,4'-DDE




Compound Name	Expected RT	Observed RT	TIC Area	Breakdown %	Pass/Fail
4,4'-DDT	8.800	8.730	3837355	1.4	Pass
4,4'-DDD	8.500	8.429	53925		
4,4'-DDE	8.200	0.000	0		

Tune Evaluation Report

+ Scan (rt: 6.425 min) Jan1001.D Pentachlorophenol



+ Scan (rt: 7.958 min) Jan1001.D Benzidine




Compound Name	Expected RT	Observed RT	Tailing Factor	PGF	Pass/Fail
Pentachlorophenol	6.800	6.425	0.4	0.2	Pass
Benzidine	8.400	7.958	0.2	0.1	Pass

Quantitation Results Report (QT Reviewed)

Data File	Jan1002.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/10/2022 11:43:19 AM
Sample Name	10-Jan-22_CCV_2	Instrument	GCMS
Vial	2	Multiplier	1.00
DA Method File	010522 bna SIM 3.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 1.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	254870	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.953	136.0	433340	40.0000	ng/ml	0.000
M Acenaphthene-d10	8.013	164.0	258334	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.793	188.0	564864	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	417462	40.0000	ng/ml	-0.013
M Perylene-d12	18.524	264.0	283136	40.0000	ng/ml	0.000
System Monitoring Compounds						
S Nitrobenzene-d5	5.156	82.0	9992	1.7046	ng/ml	m -0.013
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 34.09%		
S 2-Fluorobiphenyl	7.264	172.0	24781	1.9268	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 38.54%		
S o-Terphenyl	10.324	230.0	18478	1.7841	ng/ml	0.000
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = 35.68%		*
S Terphenyl-d14	12.288	244.0	15154	1.9618	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 39.24%		
Target Compounds						
T Naphthalene	5.966	128.0	27694	1.9033	ng/ml	96
T 2-Methylnaphthalene	6.802	141.0	15722	1.8735	ng/ml	90
T 1-Methylnaphthalene	6.902	141.0	16742	2.1576	ng/ml	95
T Acenaphthylene	7.838	152.0	27257	1.9729	ng/ml	97
T Acenaphthene	8.050	154.0	18166	1.8085	ng/ml	98
T Fluorene	8.686	166.0	21905	1.9058	ng/ml	98
T Phenanthrene	9.817	178.0	32458	1.8913	ng/ml	92
T Anthracene	9.879	178.0	28183	2.0565	ng/ml	100
T Fluoranthene	11.435	202.0	34973	1.8164	ng/ml	99
T Pyrene	11.818	202.0	38239	1.8362	ng/ml	99
T Benzo(a)Anthracene	14.726	228.0	22778	1.7900	ng/ml	99
T Chrysene	14.813	228.0	33574	1.9565	ng/ml	99
T Benzo(b)fluoranthene	17.746	252.0	19658	1.6103	ng/ml	m 98




Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	17.820	252.0	22933	1.8459	ng/ml	97
T Benzo(a)pyrene	18.400	252.0	15889	1.8651	ng/ml	99
T Indeno(1,2,3-cd)pyrene	20.254	276.0	14224	1.6778	ng/ml	94
T Dibenzo(a,h)anthracene	20.316	278.0	17462	1.7729	ng/ml	96
T Benzo(g,h,i)perylene	20.587	276.0	20939	1.7390	ng/ml	94




(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	1.7046	5.16	-0.01	9992 (m)	54.0	29.5	21.6	40.2
					128.0	32.9	21.3	39.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	1.9033	5.97	-0.01	27694	102.0	18.1	0.0	46.6
					129.0	10.9	7.6	14.1




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	1.8735	6.80	0.00	15722	142.0	136.9	103.3	191.8
					115.0	62.1	36.8	68.3




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	2.1576	6.90	0.00	16742	142.0	117.8	77.9	144.7
					115.0	62.0	44.4	82.5




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	1.9268	7.26	0.00	24781	171.0	36.5	26.4	49.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthylene	1.9729	7.84	0.00	27257	153.0	13.4	10.2	18.9






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	1.8085	8.05	0.00	18166	153.0	113.9	80.3	149.2
					152.0	52.5	38.4	71.4






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene	1.9058	8.69	0.00	21905	165.0 167.0	98.1 13.3	67.5 7.9	125.3 14.6






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Phenanthrene	1.8913	9.82	0.00	32458	176.0	18.9	10.9	20.2



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Anthracene	2.0565	9.88	0.00	28183	176.0	16.5	11.6	21.6




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
o-Terphenyl	1.7841	10.32	0.00	18478	229.0 215.0	67.7 42.9	46.7 30.2	86.8 56.2




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluoranthene	1.8164	11.44	0.00	34973	101.0	10.9	8.0	14.8




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Pyrene	1.8362	11.82	0.00	38239	101.0	13.5	9.7	18.1















Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	1.9618	12.29	0.00	15154	122.0	15.9	9.6	17.9












Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)Anthracene	1.7900	14.73	0.00	22778	226.0	27.2	19.5	36.3
					229.0	23.1	16.5	30.6



Quantitation Results Report (QT Reviewed)

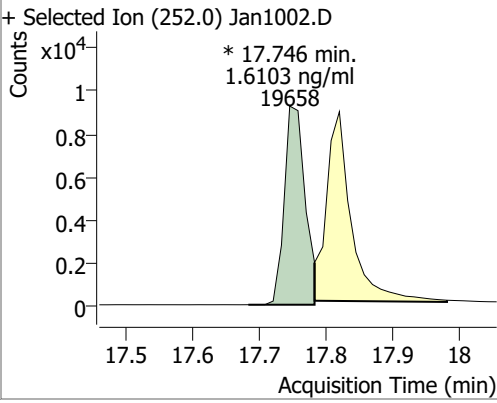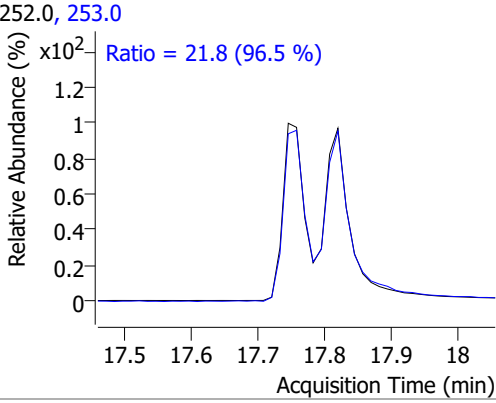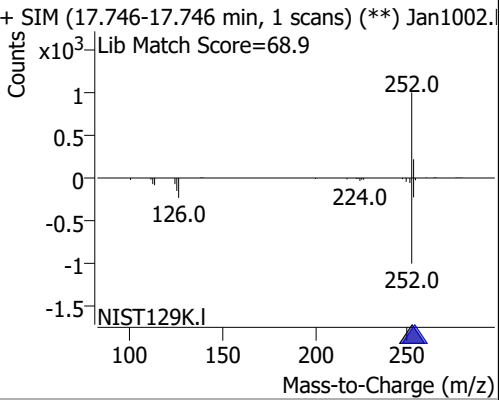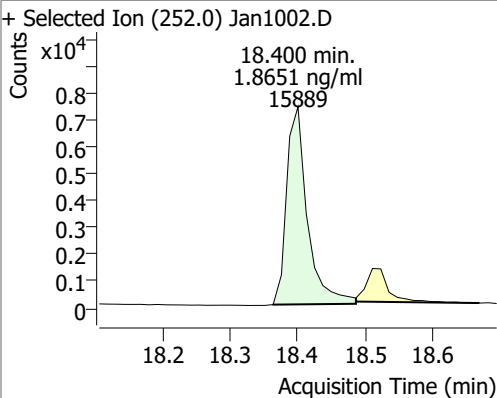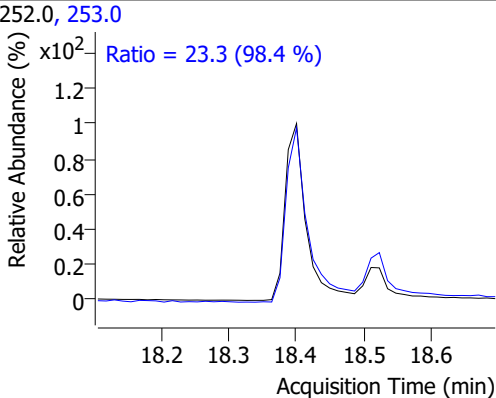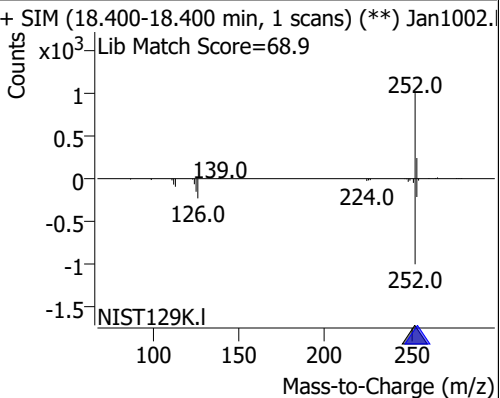Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	1.9565	14.81	-0.01	33574	226.0 229.0	31.0 21.9	22.2 15.5	41.2 28.9
+ Selected Ion (228.0) Jan1002.D 			228.0, 226.0, 229.0 			+ SIM (14.813-14.813 min, 1 scans) (**) Jan1002. Lib Match Score=51.7 		
Benzo(b)fluoranthene	1.6103	17.75	-0.01	19658 (m)	253.0	21.8	15.8	29.4
+ Selected Ion (252.0) Jan1002.D 			252.0, 253.0 			+ SIM (17.746-17.746 min, 1 scans) (**) Jan1002. Lib Match Score=68.9 		
Benzo(k)fluoranthene	1.8459	17.82	0.00	22933	253.0	24.3	16.1	30.0
+ Selected Ion (252.0) Jan1002.D 			252.0, 253.0 			+ SIM (17.820-17.820 min, 1 scans) (**) Jan1002. Lib Match Score=68.9 		
Benzo(a)pyrene	1.8651	18.40	0.00	15889	253.0	23.3	16.6	30.8
+ Selected Ion (252.0) Jan1002.D 			252.0, 253.0 			+ SIM (18.400-18.400 min, 1 scans) (**) Jan1002. Lib Match Score=68.9 		


Quantitation Results Report (QT Reviewed)

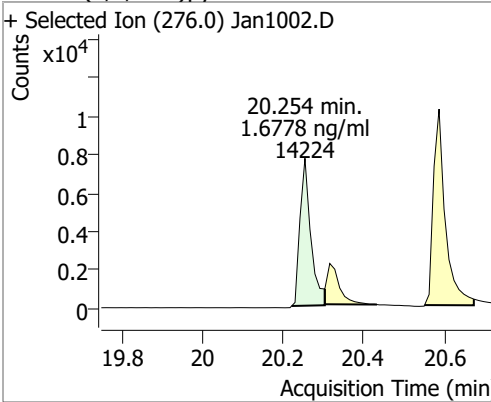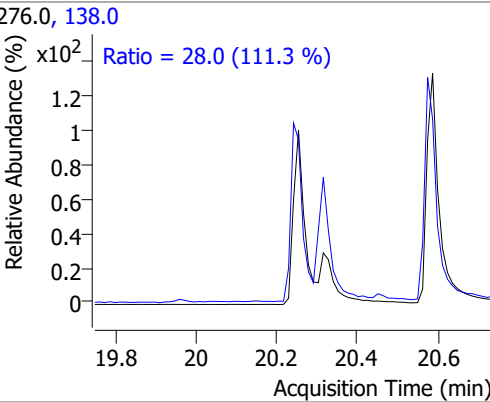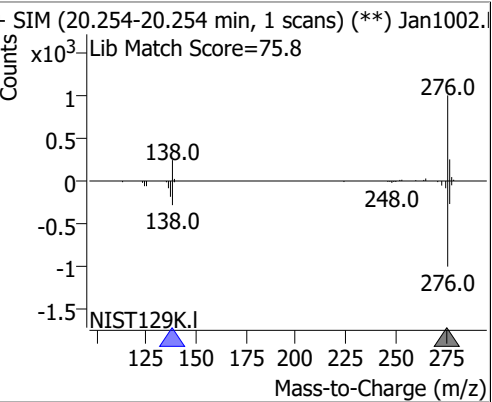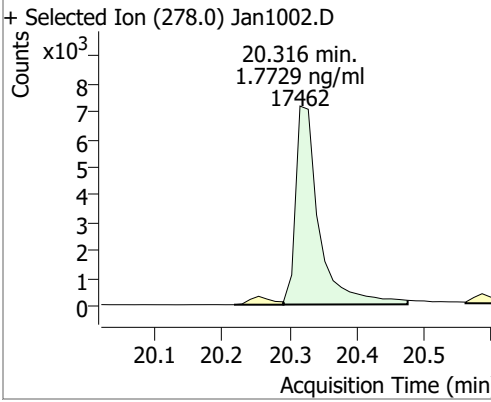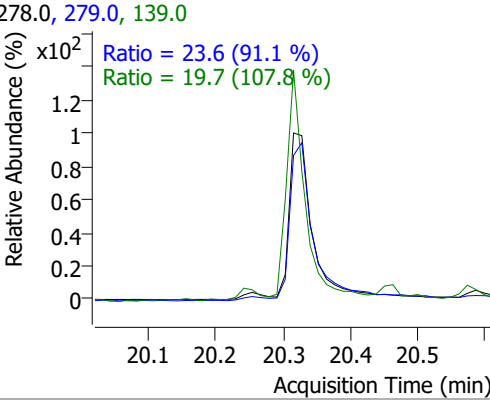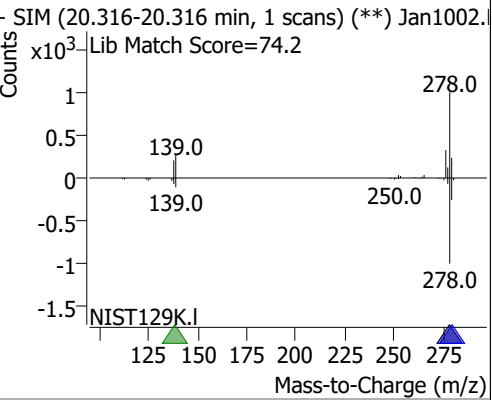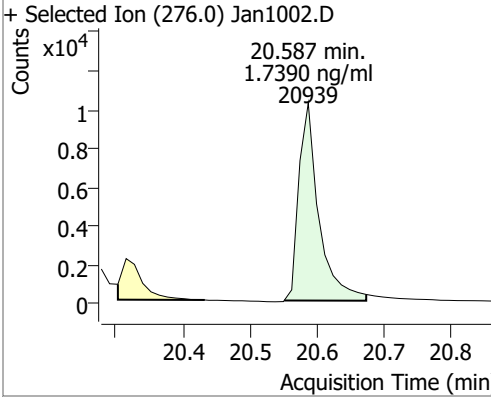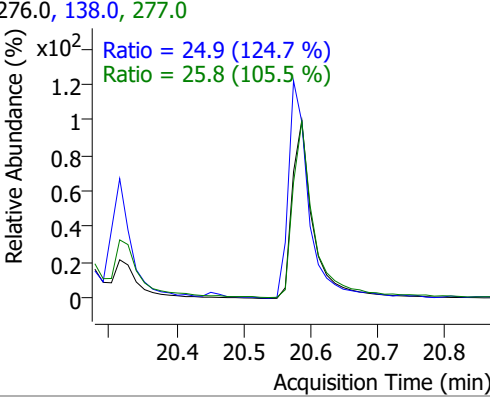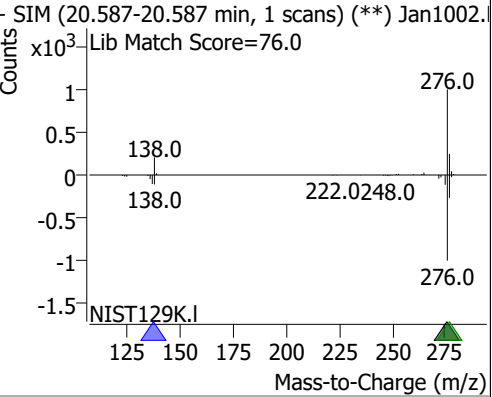Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Indeno(1,2,3-cd)pyrene	1.6778	20.25	0.01	14224	138.0	28.0	17.6	32.7
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1002.D</p>  </div> <div style="width: 30%;"> <p>276.0, 138.0</p> <p>Ratio = 28.0 (111.3 %)</p>  </div> <div style="width: 30%;"> <p>+ SIM (20.254-20.254 min, 1 scans) (**) Jan1002.D</p> <p>Lib Match Score=75.8</p>  </div> </div>								
Dibenzo(a,h)anthracene	1.7729	20.32	0.00	17462	279.0	23.6	18.1	33.6
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (278.0) Jan1002.D</p>  </div> <div style="width: 30%;"> <p>278.0, 279.0, 139.0</p> <p>Ratio = 23.6 (91.1 %)</p> <p>Ratio = 19.7 (107.8 %)</p>  </div> <div style="width: 30%;"> <p>+ SIM (20.316-20.316 min, 1 scans) (**) Jan1002.D</p> <p>Lib Match Score=74.2</p>  </div> </div>								
Benzo(g,h,i)perylene	1.7390	20.59	0.01	20939	277.0	25.8	17.1	31.8
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1002.D</p>  </div> <div style="width: 30%;"> <p>276.0, 138.0, 277.0</p> <p>Ratio = 24.9 (124.7 %)</p> <p>Ratio = 25.8 (105.5 %)</p>  </div> <div style="width: 30%;"> <p>+ SIM (20.587-20.587 min, 1 scans) (**) Jan1002.D</p> <p>Lib Match Score=76.0</p>  </div> </div>								

Quantitation Results Report (QT Reviewed)

Data File	Jan1003.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/10/2022 12:15:35 PM
Sample Name	10-Jan-22_ISTBLK_3	Instrument	GCMS
Vial	3	Multiplier	1.00
DA Method File	010522 bna SIM 3.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 1.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	224688	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	409851	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	256175	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.793	188.0	563881	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	404924	40.0000	ng/ml	-0.012
M Perylene-d12	18.524	264.0	284156	40.0000	ng/ml	0.000
System Monitoring Compounds						
S Nitrobenzene-d5	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = NA%		
S 2-Fluorobiphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = NA%		
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = NA%		
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.050	154.0	0	ng/ml	md	1
T Fluorene	0.000		0	N.D.		
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.751	228.0	0	ng/ml	md	1
T Chrysene	14.814	228.0	0	ng/ml	md	1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.413	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Nitrobenzene-d5	N.D.	5.17	54.0	30.9	128.0	30.4




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5











Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4







Quantitation Results Report (QT Reviewed)

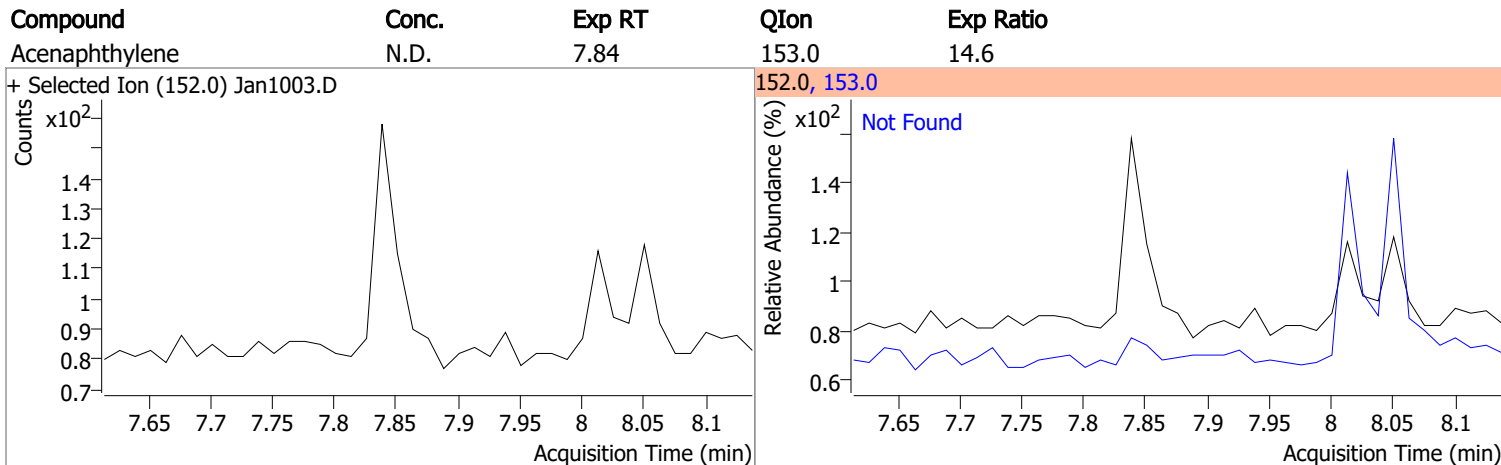

Quantitation Results Report (QT Reviewed)

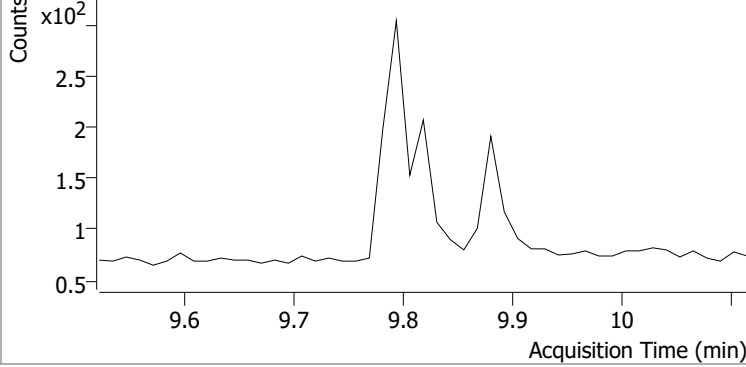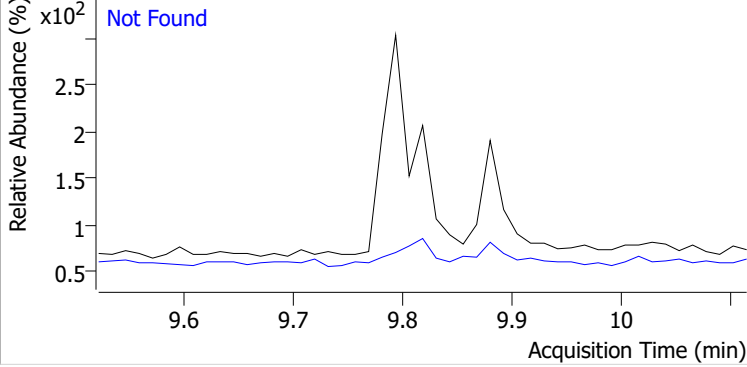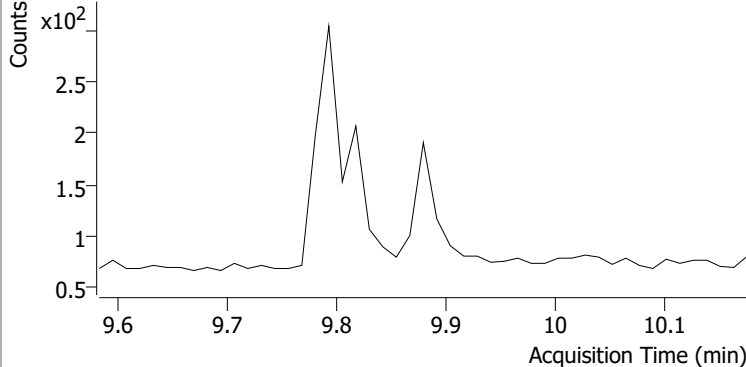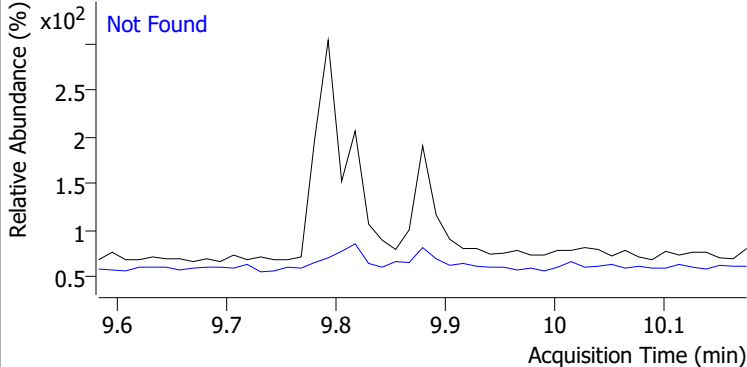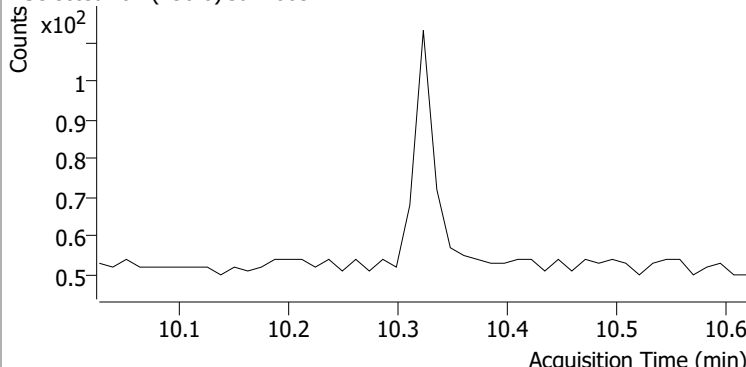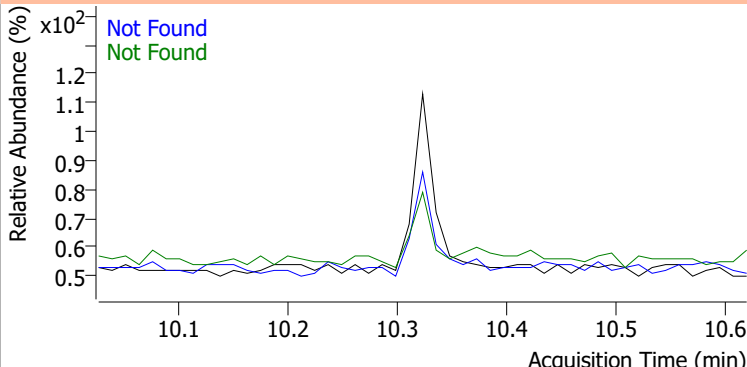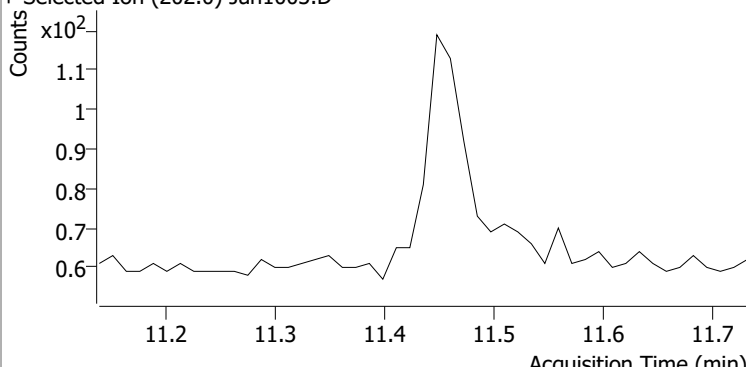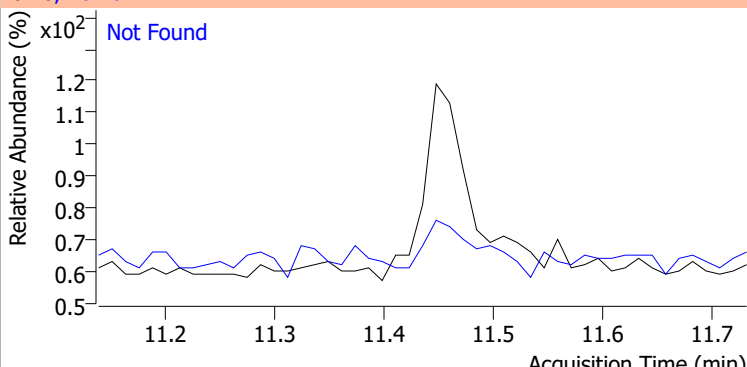
Compound	Conc.	Exp RT	QIon	Exp Ratio
Phenanthrene	N.D.	9.82	176.0	15.5
+ Selected Ion (178.0) Jan1003.D			178.0, 176.0	
				
Anthracene	N.D.	9.88	176.0	16.6
+ Selected Ion (178.0) Jan1003.D			178.0, 176.0	
				
o-Terphenyl	N.D.	10.32	229.0	66.8
+ Selected Ion (230.0) Jan1003.D			230.0, 229.0, 215.0	
				
Fluoranthene	N.D.	11.44	101.0	11.4
+ Selected Ion (202.0) Jan1003.D			202.0, 101.0	
				

Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.6	30.8




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1004.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/10/2022 12:48:04 PM
Sample Name	MB-162577	Instrument	GCMS
Vial	4	Multiplier	1.00
DA Method File	010522 bna SIM 3.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 1.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	224303	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	417537	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	259805	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.793	188.0	583481	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	429312	40.0000	ng/ml	-0.013
M Perylene-d12	18.524	264.0	292536	40.0000	ng/ml	0.000
System Monitoring Compounds						
S Nitrobenzene-d5	5.143	82.0	455014	42.5763	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 851.53%		*
S 2-Fluorobiphenyl	7.264	172.0	661811	51.1671	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1023.34%		*
S o-Terphenyl	10.324	230.0	1900	0.1776	ng/ml	0.000
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = 3.55%		*
S Terphenyl-d14	12.300	244.0	937680	118.0376	ng/ml	0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 2360.75%		*
Target Compounds						
T Naphthalene	0.000		0	N.D.		QValue
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.050	154.0	0		ng/ml	md
T Fluorene	8.686	166.0	0		ng/ml	md
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.751	228.0	0		ng/ml	md
T Chrysene	14.813	228.0	0		ng/ml	md
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.400	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	42.5763	5.14	-0.03	455014	54.0	34.8	21.6	40.2
					128.0	31.4	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4




Quantitation Results Report (QT Reviewed)

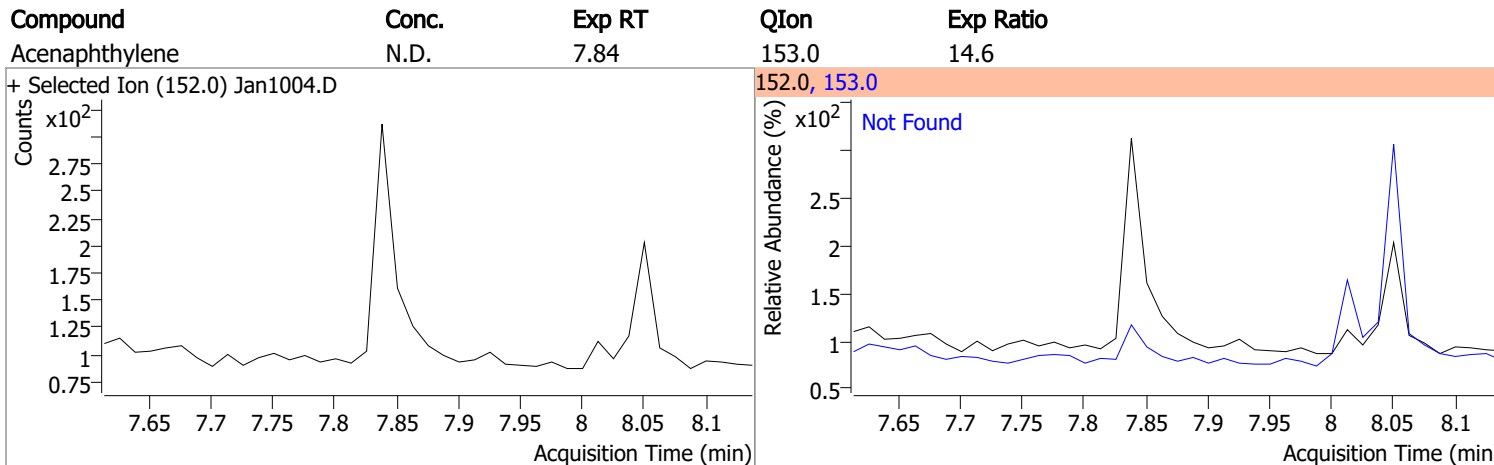


Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Phenanthrene	N.D.	9.82	176.0	15.5




Compound	Conc.	Exp RT	QIon	Exp Ratio
Anthracene	N.D.	9.88	176.0	16.6







Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
o-Terphenyl	0.1776	10.32	0.00	1900	229.0	77.1	46.7	86.8
					215.0	49.6	30.2	56.2



Compound	Conc.	Exp RT	QIon	Exp Ratio
Fluoranthene	N.D.	11.44	101.0	11.4




Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.6	30.8




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1005.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/10/2022 1:20:28 PM
Sample Name	MB-162577	Instrument	GCMS
Vial	5	Multiplier	20.00
DA Method File	010522 bna SIM 3.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 1.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	200008	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	410270	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	268401	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.793	188.0	573713	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	428519	40.0000	ng/ml	-0.013
M Perylene-d12	18.524	264.0	291518	40.0000	ng/ml	0.000
System Monitoring Compounds						
S Nitrobenzene-d5	5.156	82.0	14087	59.0423	ng/ml	-0.013
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 1180.85% *		
S 2-Fluorobiphenyl	7.265	172.0	28561	42.7488	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 854.98% *		
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.288	244.0	38203	96.3605	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 1927.21% *		
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.050	154.0	0		ng/ml md	1
T Fluorene	0.000		0	N.D.		
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.751	228.0	0		ng/ml md	1
T Chrysene	14.751	228.0	0		ng/ml md	1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.512	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	59.0423	5.16	-0.01	14087	54.0	29.2	21.6	40.2
					128.0	32.7	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	42.7488	7.26	0.00	28561	171.0	36.4	26.4	49.0




Compound	Conc.	Exp RT	QIon	Exp Ratio
Acenaphthylene	N.D.	7.84	153.0	14.6



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	N.D.	0	0	0	153.0	80.3	80.3	149.2
					152.0	38.4	38.4	71.4




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Fluorene	N.D.	8.69	165.0	96.4	167.0	11.3




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Phenanthrene	N.D.	9.82	176.0	15.5




Compound	Conc.	Exp RT	QIon	Exp Ratio
Anthracene	N.D.	9.88	176.0	16.6







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
o-Terphenyl	N.D.	10.32	229.0	66.8	215.0	43.2



Compound	Conc.	Exp RT	QIon	Exp Ratio
Fluoranthene	N.D.	11.44	101.0	11.4




Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.6	30.8




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1006.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/10/2022 1:53:00 PM
Sample Name	LLCS-162577	Instrument	GCMS
Vial	6	Multiplier	1.00
DA Method File	010522 bna SIM 3.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 1.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	245667	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	441469	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	265952	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.793	188.0	577883	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	440211	40.0000	ng/ml	-0.012
M Perylene-d12	18.524	264.0	304821	40.0000	ng/ml	0.000
System Monitoring Compounds						
S Nitrobenzene-d5	5.143	82.0	20528	3.4555	ng/ml	-0.025
Spiked Amount: 5.000		Range: 19.0 - 102.0%		Recovery = 69.11%		
S 2-Fluorobiphenyl	7.265	172.0	49652	3.7501	ng/ml	0.000
Spiked Amount: 5.000		Range: 25.0 - 94.0%		Recovery = 75.00%		
S o-Terphenyl	10.324	230.0	43271	4.0837	ng/ml	0.000
Spiked Amount: 5.000		Range: 40.0 - 140.0%		Recovery = 81.67%		
S Terphenyl-d14	12.288	244.0	40813	5.0105	ng/ml	0.000
Spiked Amount: 5.000		Range: 39.0 - 106.0%		Recovery = 100.21%		
Target Compounds						
T Naphthalene	5.966	128.0	42241	2.8495	ng/ml	99
T 2-Methylnaphthalene	6.790	141.0	25759	3.0130	ng/ml	95
T 1-Methylnaphthalene	6.902	141.0	24811	3.1385	ng/ml	95
T Acenaphthylene	7.839	152.0	48667	3.4217	ng/ml	100
T Acenaphthene	8.050	154.0	33633	3.2525	ng/ml	97
T Fluorene	8.674	166.0	47703	4.0313	ng/ml	98
T Phenanthrene	9.817	178.0	76447	4.3865	ng/ml	91
T Anthracene	9.879	178.0	69439	4.7558	ng/ml	94
T Fluoranthene	11.436	202.0	88355	4.4854	ng/ml	100
T Pyrene	11.806	202.0	99285	4.5212	ng/ml	96
T Benzo(a)Anthracene	14.714	228.0	62055	4.6843	ng/ml	99
T Chrysene	14.814	228.0	88163	4.8230	ng/ml	98
T Benzo(b)fluoranthene	17.746	252.0	57484	4.3738	ng/ml	98


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	17.807	252.0	60272	4.3058	ng/ml	100
T Benzo(a)pyrene	18.388	252.0	43815	4.4546	ng/ml	100
T Indeno(1,2,3-cd)pyrene	20.242	276.0	41018	4.4939	ng/ml	100
T Dibenzo(a,h)anthracene	20.316	278.0	50043	4.7195	ng/ml	99
T Benzo(g,h,i)perylene	20.575	276.0	64418	4.6399	ng/ml	99


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	3.4555	5.14	-0.02	20528	54.0	36.0	21.6	40.2
					128.0	27.2	21.3	39.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	2.8495	5.97	-0.01	42241	102.0	15.2	0.0	46.6
					129.0	11.2	7.6	14.1






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	3.0130	6.79	-0.01	25759	142.0	152.3	103.3	191.8
					115.0	59.1	36.8	68.3






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	3.1385	6.90	0.00	24811	142.0	116.8	77.9	144.7
					115.0	58.9	44.4	82.5






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	3.7501	7.26	0.00	49652	171.0	35.7	26.4	49.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthylene	3.4217	7.84	0.00	48667	153.0	14.6	10.2	18.9






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	3.2525	8.05	0.00	33633	153.0	111.3	80.3	149.2
					152.0	54.0	38.4	71.4






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene	4.0313	8.67	-0.01	47703	165.0 167.0	98.2 13.0	67.5 7.9	125.3 14.6






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Phenanthrene	4.3865	9.82	0.00	76447	176.0	19.2	10.9	20.2



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Anthracene	4.7558	9.88	0.00	69439	176.0	19.1	11.6	21.6




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
o-Terphenyl	4.0837	10.32	0.00	43271	229.0 215.0	67.4 43.3	46.7 30.2	86.8 56.2




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluoranthene	4.4854	11.44	0.00	88355	101.0	11.3	8.0	14.8




Pyrene	4.5212	11.81	-0.01	99285	101.0	12.5	9.7	18.1
--------	--------	-------	-------	-------	-------	------	-----	------



Terphenyl-d14	5.0105	12.29	0.00	40813	122.0	15.2	9.6	17.9
---------------	--------	-------	------	-------	-------	------	-----	------




Benzo(a)Anthracene	4.6843	14.71	-0.01	62055	226.0	27.8	19.5	36.3
					229.0	22.5	16.5	30.6




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	4.8230	14.81	-0.01	88163	226.0	30.6	22.2	41.2
					229.0	21.6	15.5	28.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(b)fluoranthene	4.3738	17.75	-0.01	57484	253.0	21.9	15.8	29.4












Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(k)fluoranthene	4.3058	17.81	-0.01	60272	253.0	23.1	16.1	30.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene	4.4546	18.39	-0.01	43815	253.0	23.7	16.6	30.8




Quantitation Results Report (QT Reviewed)

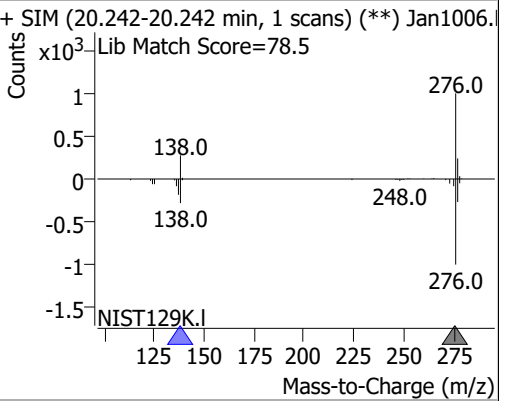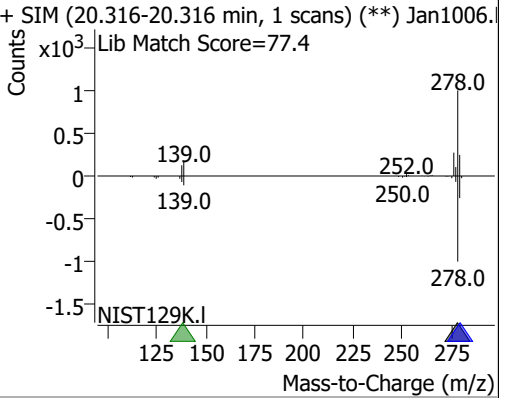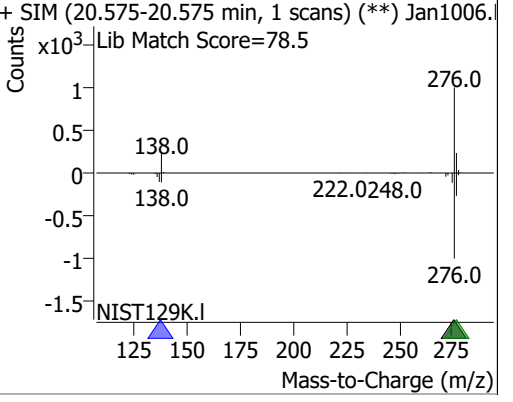Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Indeno(1,2,3-cd)pyrene	4.4939	20.24	0.00	41018	138.0	25.1	17.6	32.7
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1006.D</p>  </div> <div style="width: 30%;"> <p>276.0, 138.0</p> <p>Ratio = 25.1 (99.7 %)</p>  </div> <div style="width: 30%;"> <p>+ SIM (20.242-20.242 min, 1 scans) (**) Jan1006.D</p> <p>Lib Match Score=78.5</p>  </div> </div>								
Dibenzo(a,h)anthracene	4.7195	20.32	0.00	50043	279.0	25.3	18.1	33.6
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (278.0) Jan1006.D</p>  </div> <div style="width: 30%;"> <p>278.0, 279.0, 139.0</p> <p>Ratio = 25.3 (97.9 %)</p> <p>Ratio = 18.8 (102.7 %)</p>  </div> <div style="width: 30%;"> <p>+ SIM (20.316-20.316 min, 1 scans) (**) Jan1006.D</p> <p>Lib Match Score=77.4</p>  </div> </div>								
Benzo(g,h,i)perylene	4.6399	20.58	0.00	64418	277.0	24.5	17.1	31.8
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1006.D</p>  </div> <div style="width: 30%;"> <p>276.0, 138.0, 277.0</p> <p>Ratio = 20.8 (104.1 %)</p> <p>Ratio = 24.5 (100.0 %)</p>  </div> <div style="width: 30%;"> <p>+ SIM (20.575-20.575 min, 1 scans) (**) Jan1006.D</p> <p>Lib Match Score=78.5</p>  </div> </div>								

Quantitation Results Report (QT Reviewed)

Data File	Jan1007.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/10/2022 2:25:23 PM
Sample Name	LLCSD-162577	Instrument	GCMS
Vial	7	Multiplier	1.00
DA Method File	010522 bna SIM 3.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 1.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	214443	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	428421	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	267163	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.793	188.0	589907	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	443568	40.0000	ng/ml	-0.013
M Perylene-d12	18.524	264.0	308891	40.0000	ng/ml	0.000
System Monitoring Compounds						
S Nitrobenzene-d5	5.143	82.0	19758	3.7783	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 75.57%		
S 2-Fluorobiphenyl	7.265	172.0	49547	3.7252	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 74.50%		
S o-Terphenyl	10.324	230.0	46919	4.3377	ng/ml	0.000
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = 86.75%		
S Terphenyl-d14	12.288	244.0	43259	5.2706	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 105.41%		
Target Compounds						
T Naphthalene	5.966	128.0	35001	2.4331	ng/ml	99
T 2-Methylnaphthalene	6.790	141.0	23630	2.8482	ng/ml	90
T 1-Methylnaphthalene	6.902	141.0	22419	2.9224	ng/ml	94
T Acenaphthylene	7.839	152.0	49761	3.4827	ng/ml	99
T Acenaphthene	8.050	154.0	32582	3.1366	ng/ml	98
T Fluorene	8.673	166.0	47006	3.9544	ng/ml	98
T Phenanthrene	9.817	178.0	81717	4.5930	ng/ml	92
T Anthracene	9.879	178.0	73141	4.8951	ng/ml	96
T Fluoranthene	11.435	202.0	93492	4.6494	ng/ml	100
T Pyrene	11.806	202.0	105984	4.7897	ng/ml	97
T Benzo(a)Anthracene	14.726	228.0	65901	4.9277	ng/ml	99
T Chrysene	14.814	228.0	93718	5.0800	ng/ml	98
T Benzo(b)fluoranthene	17.746	252.0	60432	4.5376	ng/ml	99


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	17.807	252.0	65404	4.5833	ng/ml	96
T Benzo(a)pyrene	18.388	252.0	45650	4.5654	ng/ml	98
T Indeno(1,2,3-cd)pyrene	20.242	276.0	43692	4.7238	ng/ml	98
T Dibenzo(a,h)anthracene	20.316	278.0	53455	4.9748	ng/ml	98
T Benzo(g,h,i)perylene	20.575	276.0	64257	4.5749	ng/ml m	96


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	3.7783	5.14	-0.02	19758	54.0	35.4	21.6	40.2
					128.0	26.3	21.3	39.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	2.4331	5.97	-0.01	35001	102.0	15.2	0.0	46.6
					129.0	10.9	7.6	14.1




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	2.8482	6.79	-0.01	23630	142.0	159.9	103.3	191.8
					115.0	58.8	36.8	68.3




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	2.9224	6.90	0.00	22419	142.0	117.4	77.9	144.7
					115.0	59.2	44.4	82.5




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	3.7252	7.26	0.00	49547	171.0	37.0	26.4	49.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthylene	3.4827	7.84	0.00	49761	153.0	14.4	10.2	18.9






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	3.1366	8.05	0.00	32582	153.0	112.2	80.3	149.2
					152.0	54.5	38.4	71.4






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene	3.9544	8.67	-0.01	47006	165.0	98.3	67.5	125.3
					167.0	13.3	7.9	14.6






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Phenanthrene	4.5930	9.82	0.00	81717	176.0	19.0	10.9	20.2



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Anthracene	4.8951	9.88	0.00	73141	176.0	18.3	11.6	21.6




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
o-Terphenyl	4.3377	10.32	0.00	46919	229.0	67.2	46.7	86.8
					215.0	43.1	30.2	56.2




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluoranthene	4.6494	11.44	0.00	93492	101.0	11.6	8.0	14.8




Pyrene	4.7897	11.81	-0.01	105984	101.0	12.6	9.7	18.1
--------	--------	-------	-------	--------	-------	------	-----	------



Terphenyl-d14	5.2706	12.29	0.00	43259	122.0	15.2	9.6	17.9
---------------	--------	-------	------	-------	-------	------	-----	------




Benzo(a)Anthracene	4.9277	14.73	0.00	65901	226.0 229.0	27.8 22.2	19.5 16.5	36.3 30.6
--------------------	--------	-------	------	-------	----------------	--------------	--------------	--------------




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	5.0800	14.81	-0.01	93718	226.0	30.4	22.2	41.2
					229.0	21.4	15.5	28.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(b)fluoranthene	4.5376	17.75	-0.01	60432	253.0	22.0	15.8	29.4



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(k)fluoranthene	4.5833	17.81	-0.01	65404	253.0	21.0	16.1	30.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene	4.5654	18.39	-0.01	45650	253.0	24.5	16.6	30.8




Quantitation Results Report (QT Reviewed)

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Indeno(1,2,3-cd)pyrene	4.7238	20.24	0.00	43692	138.0	24.3	17.6	32.7
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1007.D</p> </div> <div style="width: 30%;"> <p>276.0, 138.0</p> <p>Ratio = 24.3 (96.7 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.242-20.242 min, 1 scans) (**) Jan1007.D</p> <p>Lib Match Score=78.6</p> </div> </div>								
Dibenzo(a,h)anthracene	4.9748	20.32	0.00	53455	279.0	24.5	18.1	33.6
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (278.0) Jan1007.D</p> </div> <div style="width: 30%;"> <p>278.0, 279.0, 139.0</p> <p>Ratio = 24.5 (94.9 %)</p> <p>Ratio = 18.5 (101.4 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.316-20.316 min, 1 scans) (**) Jan1007.D</p> <p>Lib Match Score=77.1</p> </div> </div>								
Benzo(g,h,i)perylene	4.5749	20.58	0.00	64257 (m)	277.0	26.2	17.1	31.8
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1007.D</p> </div> <div style="width: 30%;"> <p>276.0, 138.0, 277.0</p> <p>Ratio = 22.7 (113.7 %)</p> <p>Ratio = 26.2 (106.9 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.575-20.575 min, 1 scans) (**) Jan1007.D</p> <p>Lib Match Score=78.4</p> </div> </div>								

Quantitation Results Report (QT Reviewed)

Data File	Jan1008.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/10/2022 2:57:53 PM
Sample Name	B21122077-001C	Instrument	GCMS
Vial	8	Multiplier	1.00
DA Method File	010522 bna SIM 3.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 1.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	237523	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	445021	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	261960	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.793	188.0	568281	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	437360	40.0000	ng/ml	-0.013
M Perylene-d12	18.524	264.0	297154	40.0000	ng/ml	0.000
System Monitoring Compounds						
S Nitrobenzene-d5	5.143	82.0	472280	42.0234	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 840.47%		*
S 2-Fluorobiphenyl	7.264	172.0	869395	66.6633	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1333.27%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.288	244.0	843541	104.2333	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 2084.67%		*
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.050	154.0	0		ng/ml	md 1
T Fluorene	8.985	166.0	0		ng/ml	md 1
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.751	228.0	0		ng/ml	md 1
T Chrysene	14.751	228.0	0		ng/ml	md 1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.512	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	42.0234	5.14	-0.03	472280	54.0	33.9	21.6	40.2
					128.0	31.4	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5











Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4



Quantitation Results Report (QT Reviewed)

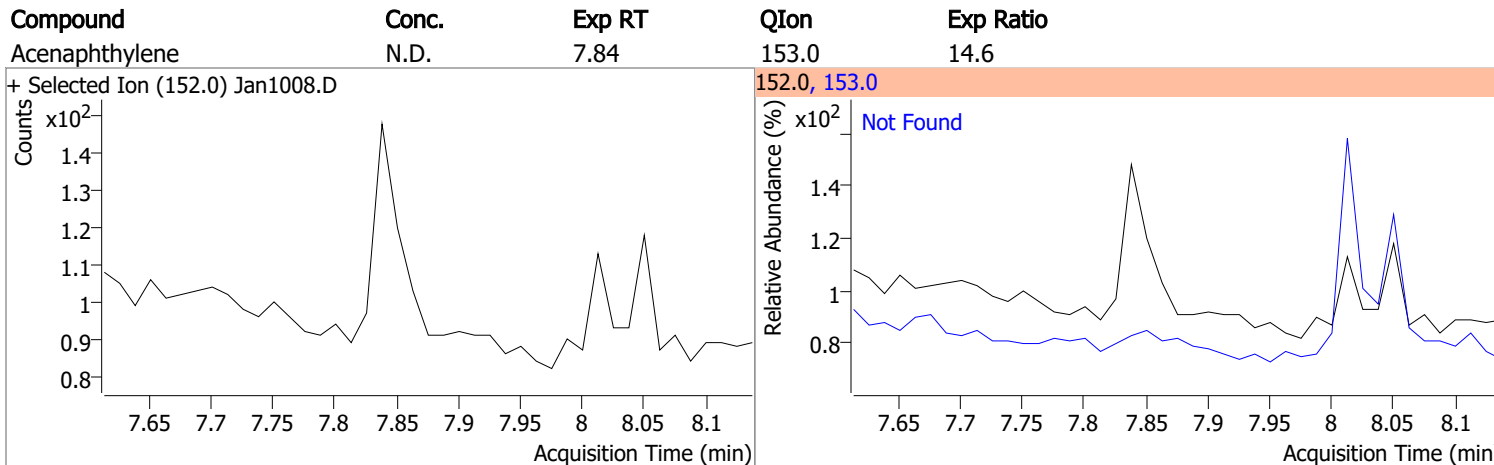


Quantitation Results Report (QT Reviewed)

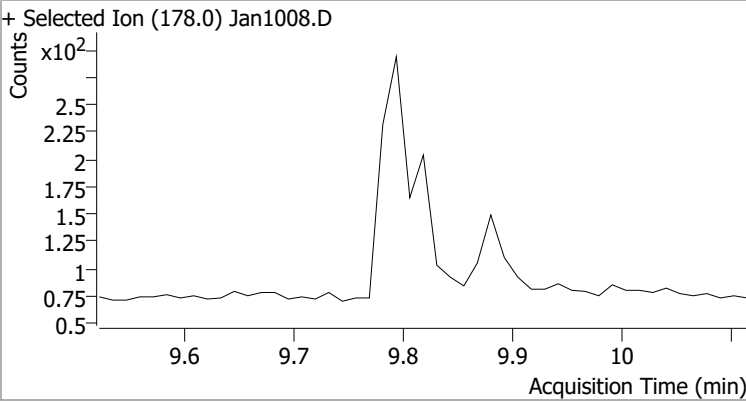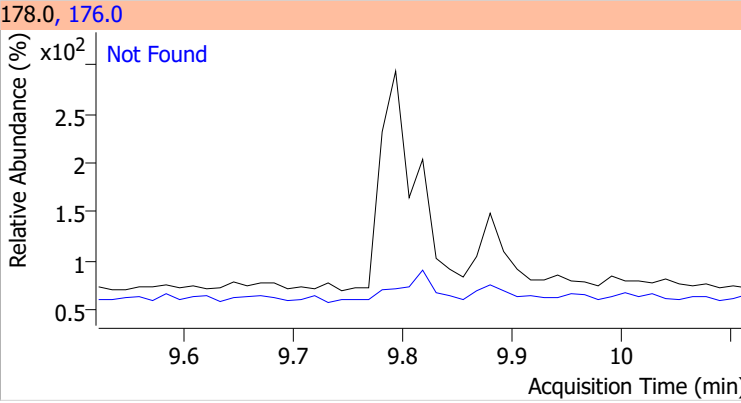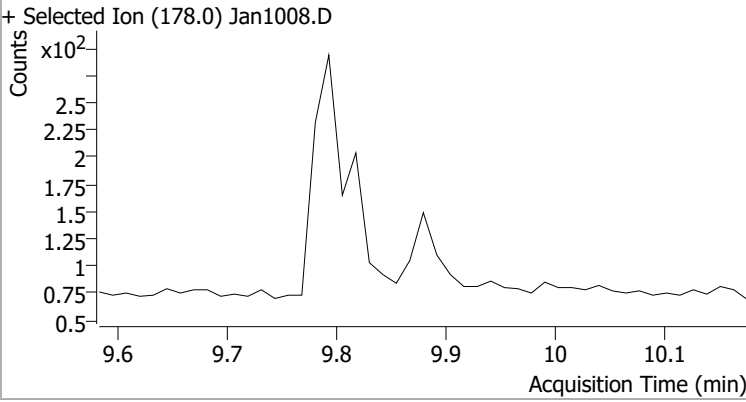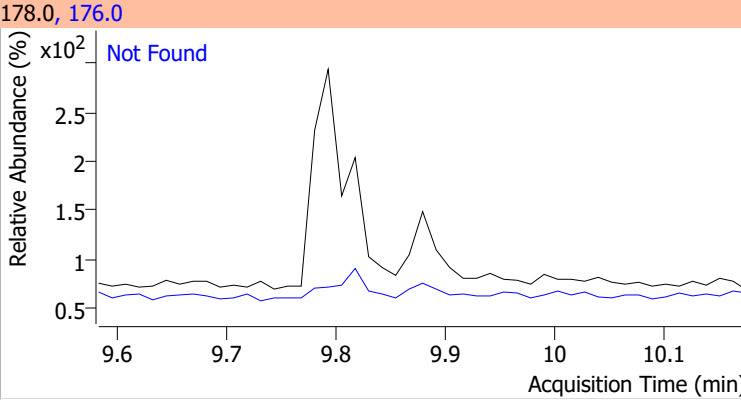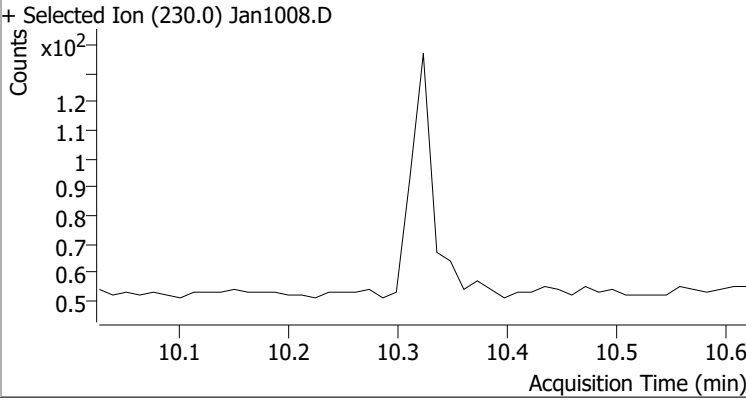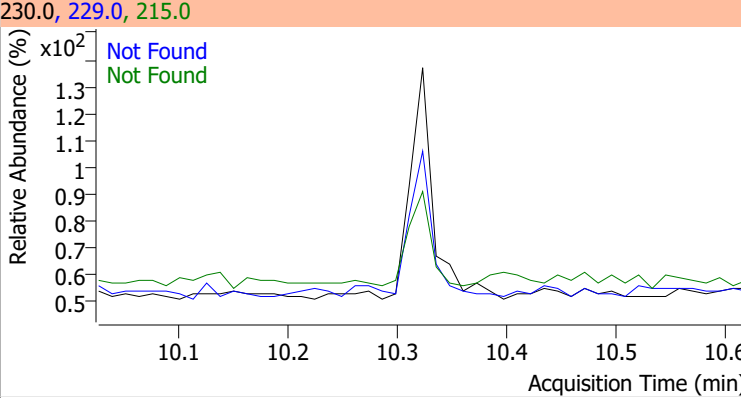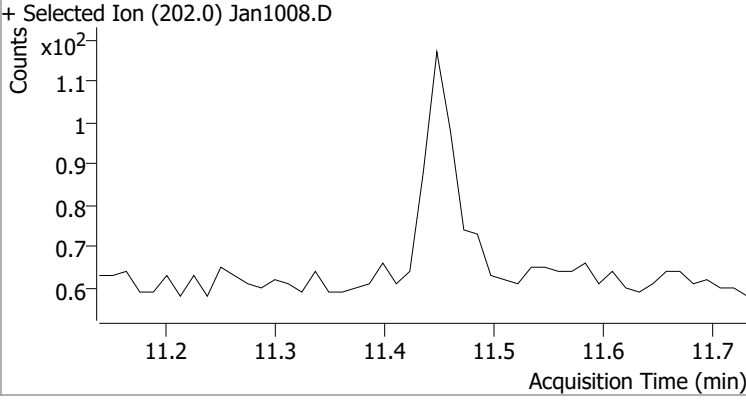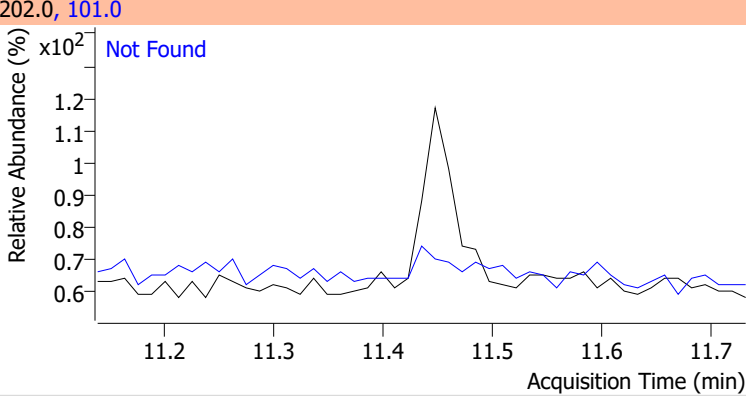
Compound	Conc.	Exp RT	QIon	Exp Ratio		
Phenanthrene	N.D.	9.82	176.0	15.5		
+ Selected Ion (178.0) Jan1008.D 			178.0, 176.0 			
Anthracene	N.D.	9.88	176.0	16.6		
+ Selected Ion (178.0) Jan1008.D 			178.0, 176.0 			
o-Terphenyl	N.D.	10.32	229.0	66.8	QIon	Exp Ratio
			215.0	43.2		
+ Selected Ion (230.0) Jan1008.D 			230.0, 229.0, 215.0 			
Fluoranthene	N.D.	11.44	101.0	11.4		
+ Selected Ion (202.0) Jan1008.D 			202.0, 101.0 			

Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Pyrene	N.D.	11.82	101.0	13.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	104.2333	12.29	0.00	843541	122.0	14.9	9.6	17.9



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)Anthracene		0		0	226.0		19.5	36.3
					229.0		16.5	30.6




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene		0		0	226.0		22.2	41.2
					229.0		15.5	28.9




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.6	30.8




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1009.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/10/2022 3:30:15 PM
Sample Name	B21122077-001C	Instrument	GCMS
Vial	9	Multiplier	20.00
DA Method File	010522 bna SIM 3.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 1.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	190336	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	405547	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	251352	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.793	188.0	526142	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	413589	40.0000	ng/ml	-0.012
M Perylene-d12	18.512	264.0	288058	40.0000	ng/ml	-0.012
System Monitoring Compounds						
S Nitrobenzene-d5	5.156	82.0	13114	57.8503	ng/ml	-0.012
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 1157.01%		*
S 2-Fluorobiphenyl	7.265	172.0	40270	64.3628	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1287.26%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.288	244.0	35825	93.6235	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 1872.47%		*
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.050	154.0	0		ng/ml	md
T Fluorene	0.000		0	N.D.		
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.751	228.0	0		ng/ml	md
T Chrysene	14.814	228.0	0		ng/ml	md
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.413	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	57.8503	5.16	-0.01	13114	54.0	31.4	21.6	40.2
					128.0	36.2	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	64.3628	7.26	0.00	40270	171.0	36.6	26.4	49.0




Compound	Conc.	Exp RT	QIon	Exp Ratio
Acenaphthylene	N.D.	7.84	153.0	14.6











Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene		0		0	153.0		80.3	149.2
					152.0		38.4	71.4



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Fluorene	N.D.	8.69	165.0	96.4	167.0	11.3




Quantitation Results Report (QT Reviewed)

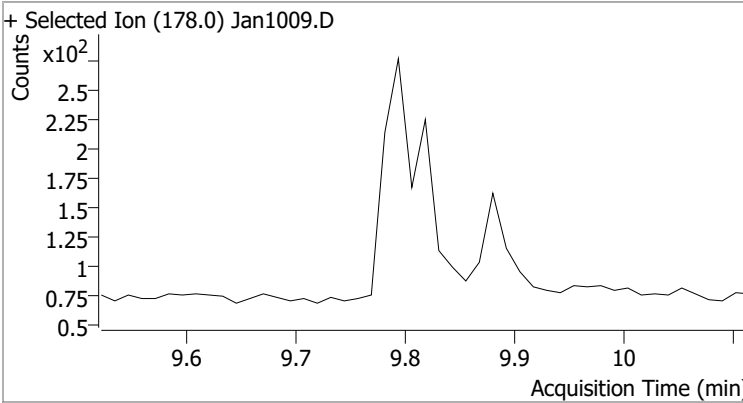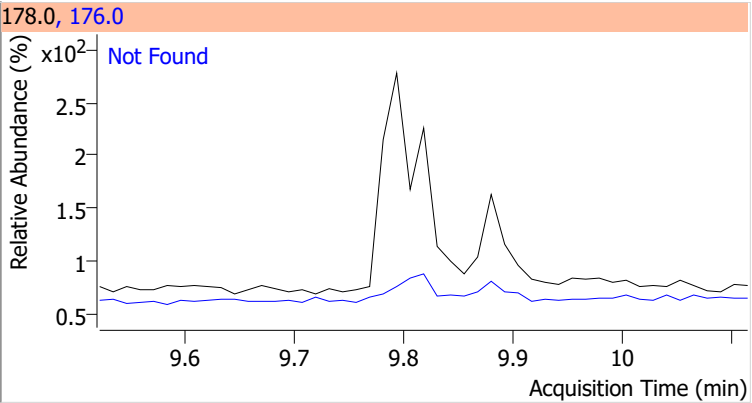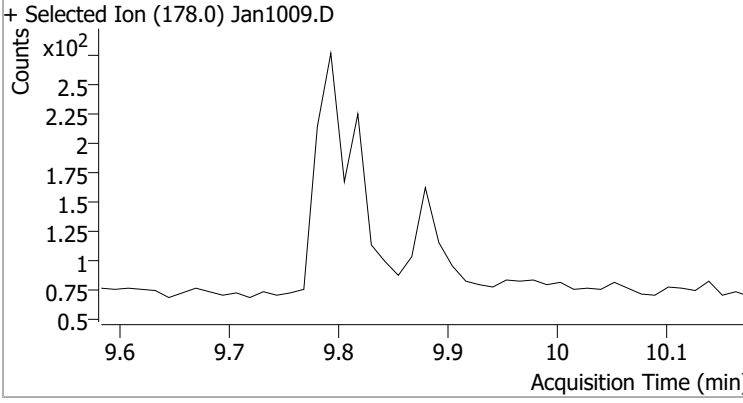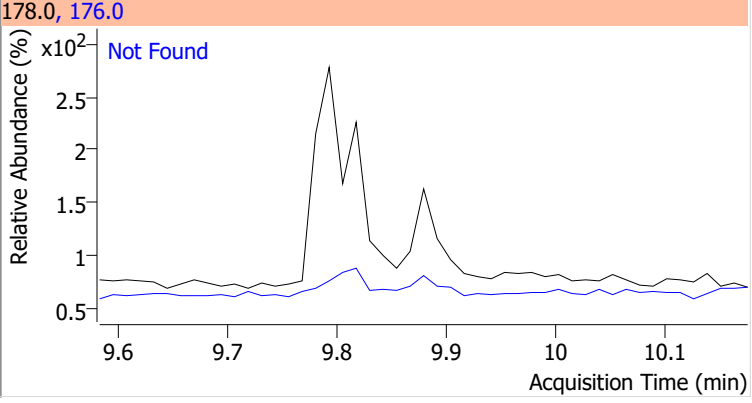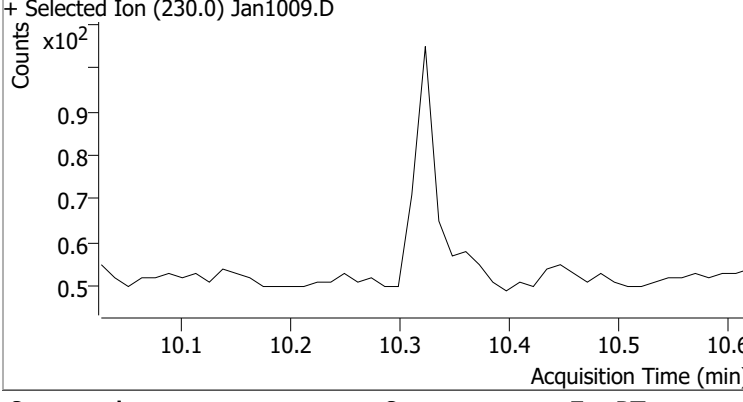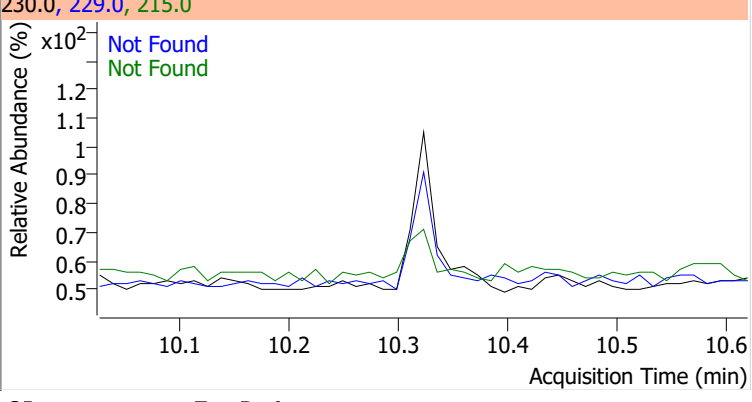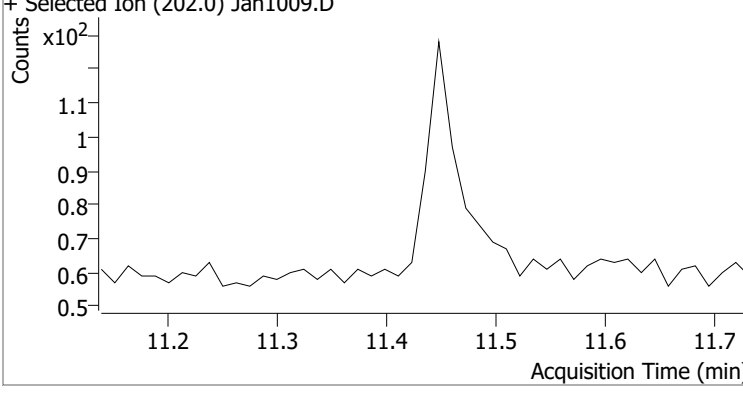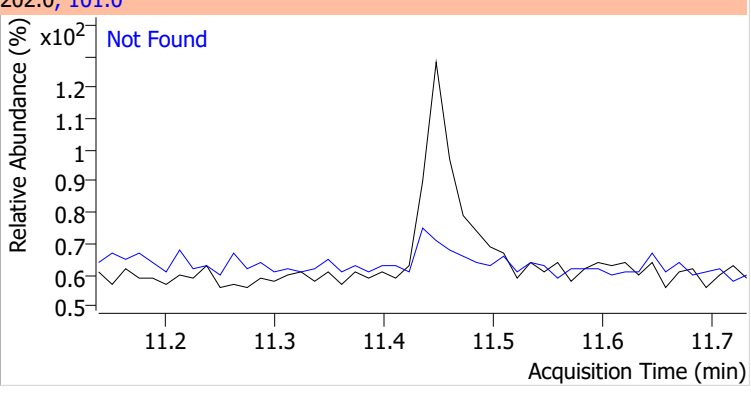
Compound	Conc.	Exp RT	QIon	Exp Ratio		
Phenanthrene	N.D.	9.82	176.0	15.5		
+ Selected Ion (178.0) Jan1009.D 			178.0, 176.0 			
Anthracene	N.D.	9.88	176.0	16.6		
+ Selected Ion (178.0) Jan1009.D 			178.0, 176.0 			
o-Terphenyl	N.D.	10.32	229.0	66.8	QIon	Exp Ratio
			215.0	43.2		
+ Selected Ion (230.0) Jan1009.D 			230.0, 229.0, 215.0 			
Fluoranthene	N.D.	11.44	101.0	11.4		
+ Selected Ion (202.0) Jan1009.D 			202.0, 101.0 			

Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Pyrene	N.D.	11.82	101.0	13.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	93.6235	12.29	0.00	35825	122.0	15.4	9.6	17.9



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)Anthracene	0	0	0	0	226.0 229.0		19.5 16.5	36.3 30.6




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	0	0	0	0	226.0 229.0		22.2 15.5	41.2 28.9




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.6	30.8




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1010.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/10/2022 4:02:43 PM
Sample Name	B21122088-001C	Instrument	GCMS
Vial	10	Multiplier	1.00
DA Method File	010522 bna SIM 3.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 1.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	257567	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	446998	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	262145	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.793	188.0	561226	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	446034	40.0000	ng/ml	-0.013
M Perylene-d12	18.512	264.0	316613	40.0000	ng/ml	-0.012
System Monitoring Compounds						
S Nitrobenzene-d5	5.143	82.0	472914	39.8824	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 797.65%		*
S 2-Fluorobiphenyl	7.265	172.0	791152	60.6209	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1212.42%		*
S o-Terphenyl	10.324	230.0	1839	0.1787	ng/ml	0.000
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = 3.57%		*
S Terphenyl-d14	12.288	244.0	848133	102.7626	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 2055.25%		*
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.050	154.0	0		ng/ml	md 1
T Fluorene	8.686	166.0	0		ng/ml	md 1
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.751	228.0	0		ng/ml	md 1
T Chrysene	14.751	228.0	0		ng/ml	md 1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.512	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	39.8824	5.14	-0.02	472914	54.0	34.1	21.6	40.2
					128.0	32.9	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4







Quantitation Results Report (QT Reviewed)

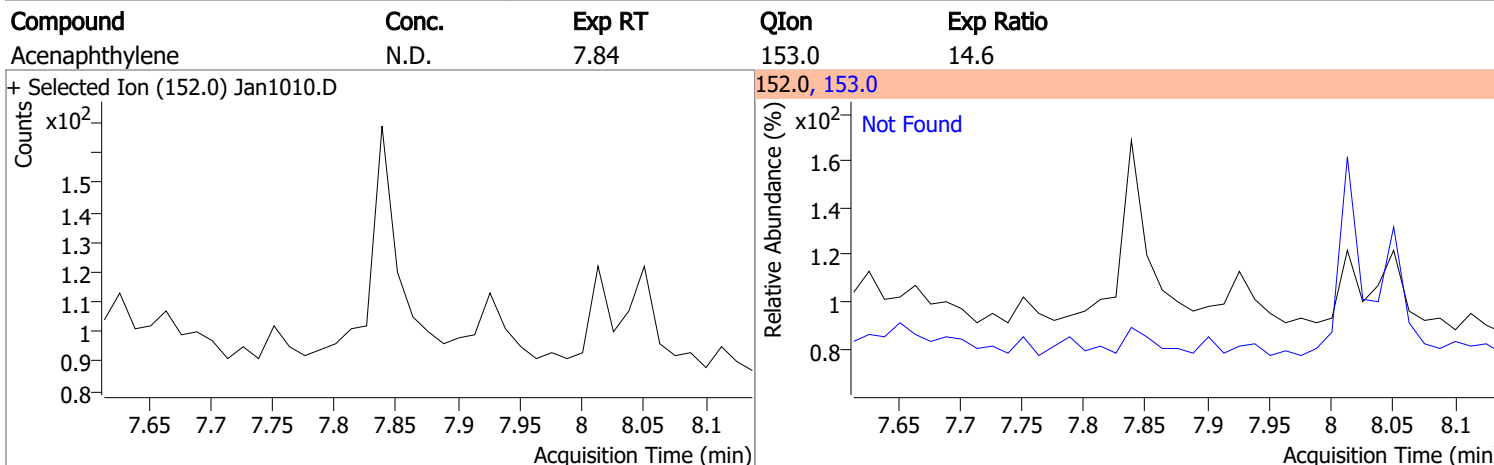

Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.6	30.8




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1011.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/10/2022 4:35:03 PM
Sample Name	B21122088-001C	Instrument	GCMS
Vial	11	Multiplier	20.00
DA Method File	010522 bna SIM 3.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 1.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	238452	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	427320	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	266037	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.793	188.0	589968	40.0000	ng/ml	0.000
M Chrysene-d12	14.764	240.0	431432	40.0000	ng/ml	0.000
M Perylene-d12	18.524	264.0	307501	40.0000	ng/ml	0.000
System Monitoring Compounds						
S Nitrobenzene-d5	5.156	82.0	17949	62.7814	ng/ml	-0.013
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 1255.63% *		
S 2-Fluorobiphenyl	7.264	172.0	40469	61.1108	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1222.22% *		
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.288	244.0	41382	103.6732	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 2073.46% *		
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.050	154.0	0		ng/ml	md 1
T Fluorene	0.000		0	N.D.		
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.751	228.0	0		ng/ml	md 1
T Chrysene	14.751	228.0	0		ng/ml	md 1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.413	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	62.7814	5.16	-0.01	17949	54.0	30.7	21.6	40.2
					128.0	35.3	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	61.1108	7.26	0.00	40469	171.0	37.5	26.4	49.0




Compound	Conc.	Exp RT	QIon	Exp Ratio
Acenaphthylene	N.D.	7.84	153.0	14.6











Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene		0		0	153.0		80.3	149.2
					152.0		38.4	71.4



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Fluorene	N.D.	8.69	165.0	96.4	167.0	11.3




Quantitation Results Report (QT Reviewed)

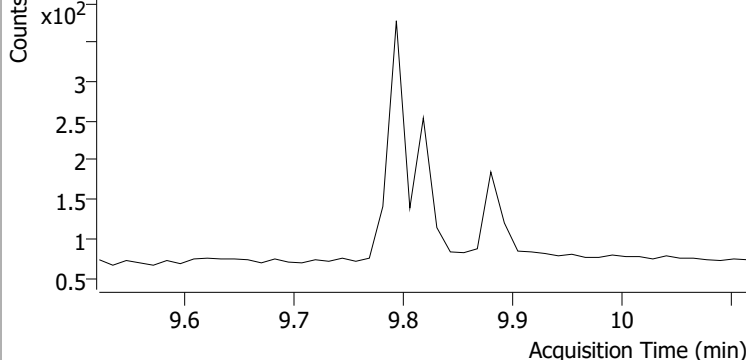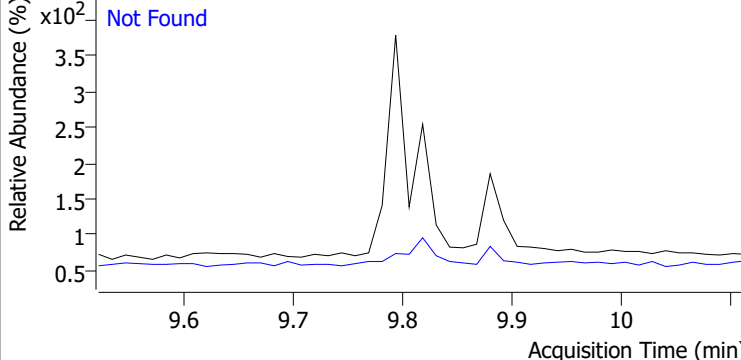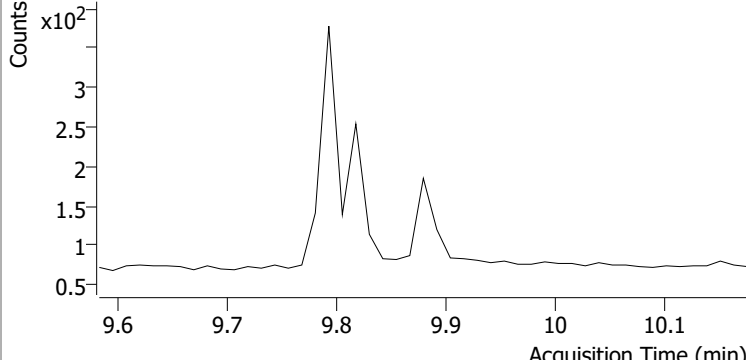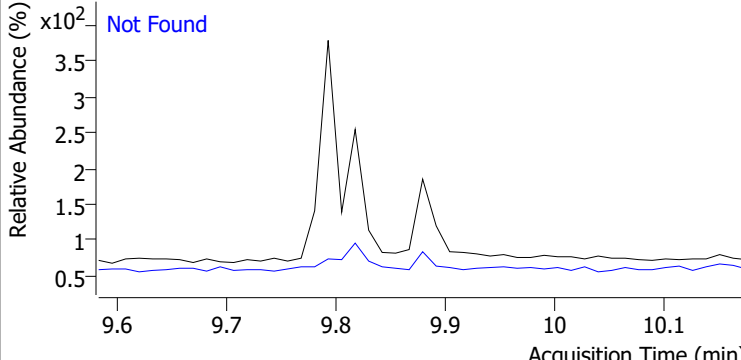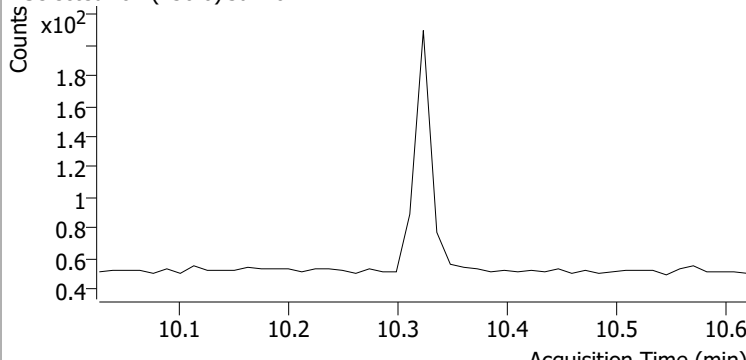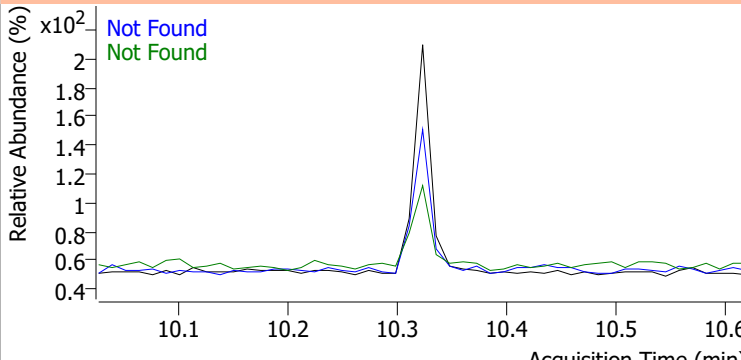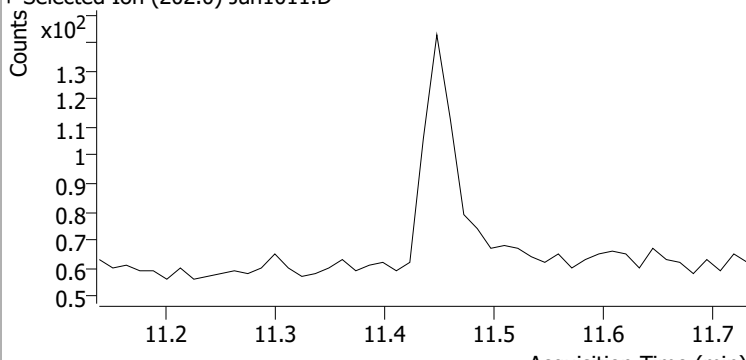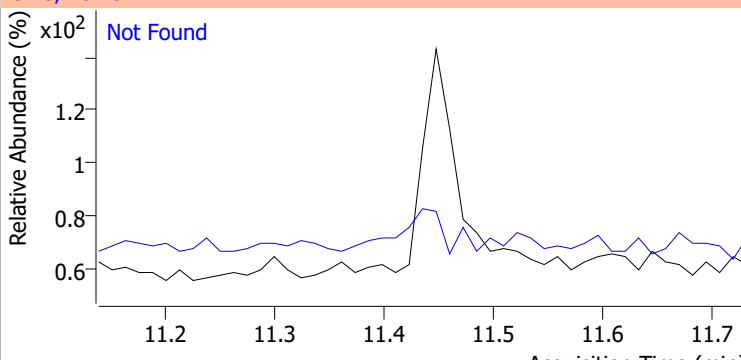
Compound	Conc.	Exp RT	QIon	Exp Ratio		
Phenanthrene	N.D.	9.82	176.0	15.5		
+ Selected Ion (178.0) Jan1011.D			178.0, 176.0			
						
Anthracene	N.D.	9.88	176.0	16.6		
+ Selected Ion (178.0) Jan1011.D			178.0, 176.0			
						
o-Terphenyl	N.D.	10.32	229.0	66.8	QIon	Exp Ratio
+ Selected Ion (230.0) Jan1011.D			230.0, 229.0, 215.0			
						
Fluoranthene	N.D.	11.44	101.0	11.4		
+ Selected Ion (202.0) Jan1011.D			202.0, 101.0			
						

Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Pyrene	N.D.	11.82	101.0	13.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	103.6732	12.29	0.00	41382	122.0	14.9	9.6	17.9



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)Anthracene	0	0	0	0	226.0		19.5	36.3
					229.0		16.5	30.6




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	0	0	0	0	226.0		22.2	41.2
					229.0		15.5	28.9




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.6	30.8




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1012.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/10/2022 5:07:25 PM
Sample Name	B21122090-001C	Instrument	GCMS
Vial	12	Multiplier	1.00
DA Method File	010522 bna SIM 3.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 1.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	229592	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	432254	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	255583	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.793	188.0	582888	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	443668	40.0000	ng/ml	-0.013
M Perylene-d12	18.524	264.0	315279	40.0000	ng/ml	0.000
System Monitoring Compounds						
S Nitrobenzene-d5	5.143	82.0	404946	38.8376	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 776.75%		*
S 2-Fluorobiphenyl	7.264	172.0	796972	62.6347	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1252.69%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.300	244.0	872455	106.2732	ng/ml	0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 2125.46%		*
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.013	154.0	0		ng/ml	md 1
T Fluorene	0.000		0	N.D.		
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.751	228.0	0		ng/ml	md 1
T Chrysene	14.751	228.0	0		ng/ml	md 1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.524	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	38.8376	5.14	-0.02	404946	54.0	32.9	21.6	40.2
					128.0	31.7	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	62.6347	7.26	0.00	796972	171.0	39.4	26.4	49.0




Compound	Conc.	Exp RT	QIon	Exp Ratio
Acenaphthylene	N.D.	7.84	153.0	14.6











Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene		0		0	153.0		80.3	149.2
					152.0		38.4	71.4







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Fluorene	N.D.	8.69	165.0	96.4	167.0	11.3



Quantitation Results Report (QT Reviewed)

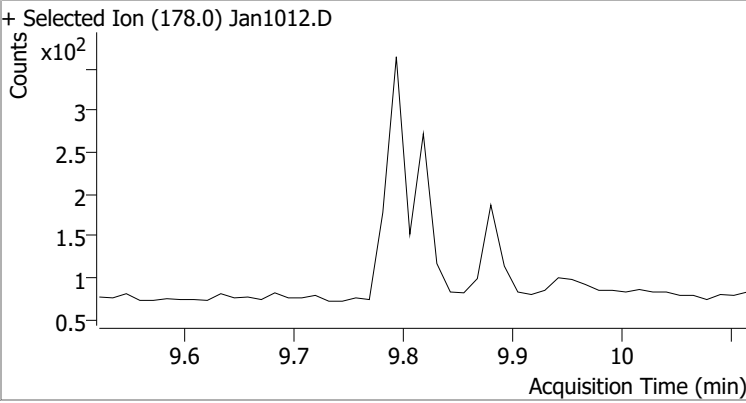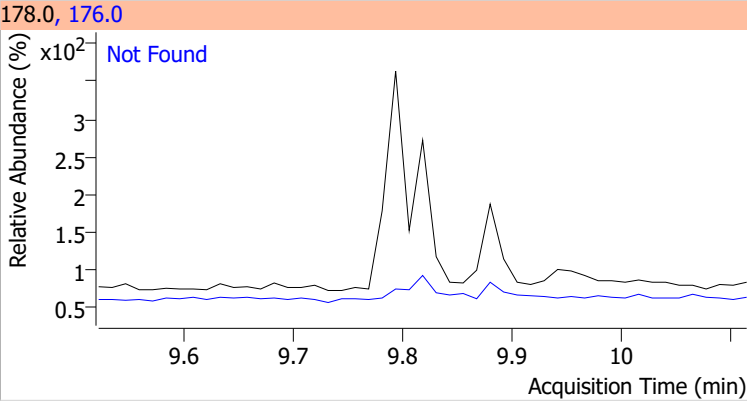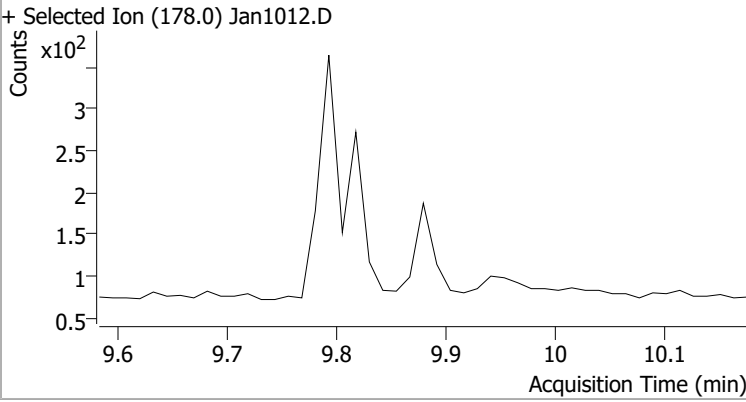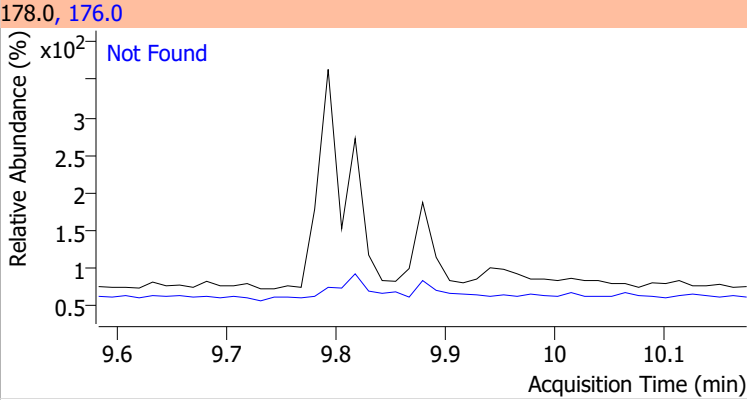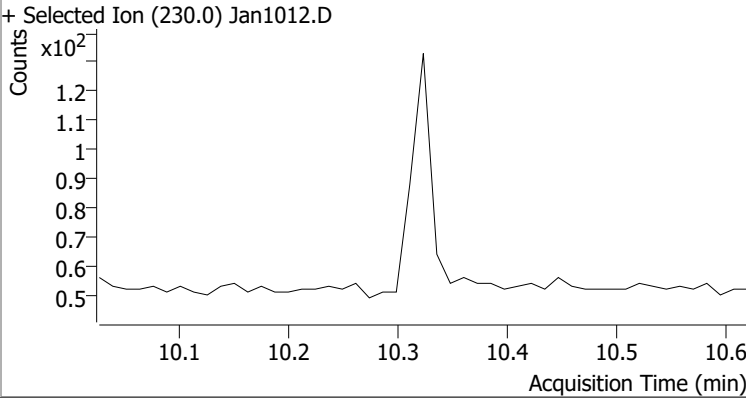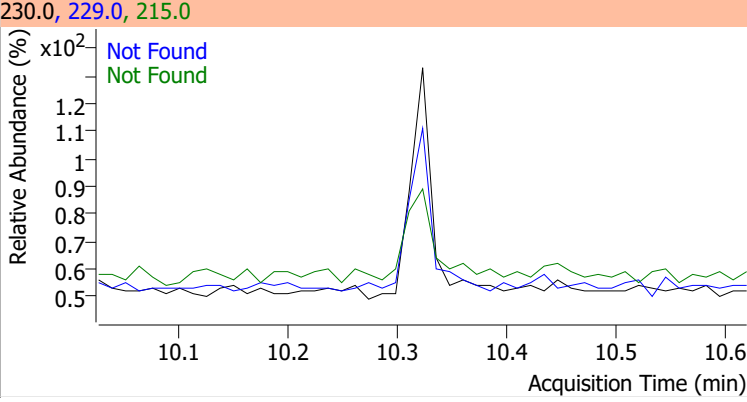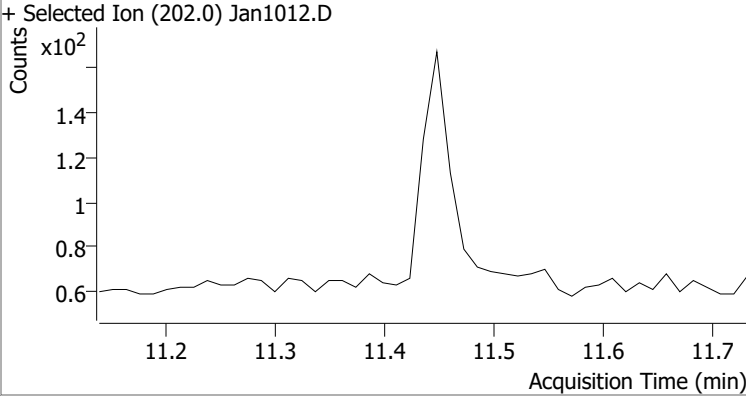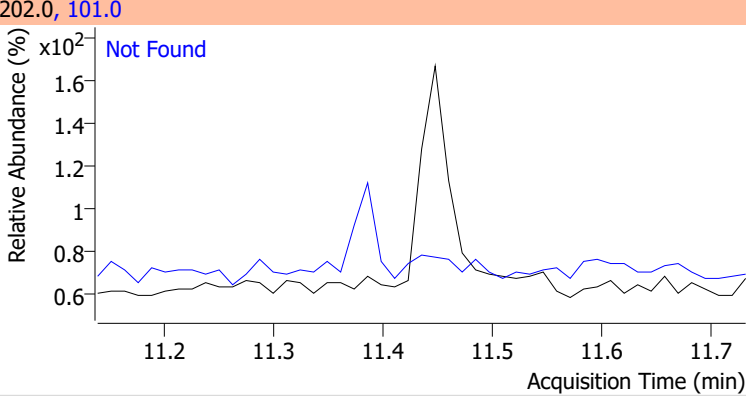
Compound	Conc.	Exp RT	QIon	Exp Ratio		
Phenanthrene	N.D.	9.82	176.0	15.5		
+ Selected Ion (178.0) Jan1012.D			178.0, 176.0			
						
Anthracene	N.D.	9.88	176.0	16.6		
+ Selected Ion (178.0) Jan1012.D			178.0, 176.0			
						
o-Terphenyl	N.D.	10.32	229.0	66.8	QIon	Exp Ratio
+ Selected Ion (230.0) Jan1012.D			230.0, 229.0, 215.0			
						
Fluoranthene	N.D.	11.44	101.0	11.4		
+ Selected Ion (202.0) Jan1012.D			202.0, 101.0			
						

Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.6	30.8




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1013.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/10/2022 5:39:43 PM
Sample Name	B21122090-001C	Instrument	GCMS
Vial	13	Multiplier	20.00
DA Method File	010522 bna SIM 3.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 1.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	232219	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	421277	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	247219	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.792	188.0	564284	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	426384	40.0000	ng/ml	-0.013
M Perylene-d12	18.524	264.0	304317	40.0000	ng/ml	0.000
System Monitoring Compounds						
S Nitrobenzene-d5	5.155	82.0	14218	51.8388	ng/ml	-0.013
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 1036.78% *		
S 2-Fluorobiphenyl	7.264	172.0	39978	64.9636	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1299.27% *		
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.288	244.0	38292	97.0674	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 1941.35% *		
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.050	154.0	0		ng/ml	md 1
T Fluorene	0.000		0	N.D.		
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.751	228.0	0		ng/ml	md 1
T Chrysene	14.751	228.0	0		ng/ml	md 1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.413	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	51.8388	5.16	-0.01	14218	54.0 128.0	29.9 34.2	21.6 21.3	40.2 39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	64.9636	7.26	0.00	39978	171.0	36.3	26.4	49.0




Compound	Conc.	Exp RT	QIon	Exp Ratio
Acenaphthylene	N.D.	7.84	153.0	14.6











Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene		0		0	153.0		80.3	149.2
					152.0		38.4	71.4







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Fluorene	N.D.	8.69	165.0	96.4	167.0	11.3



Quantitation Results Report (QT Reviewed)

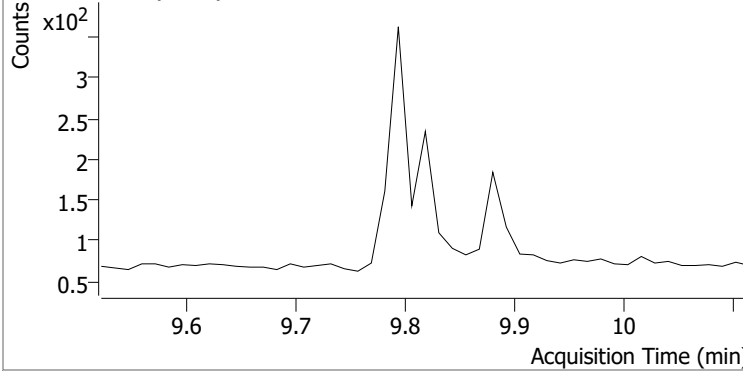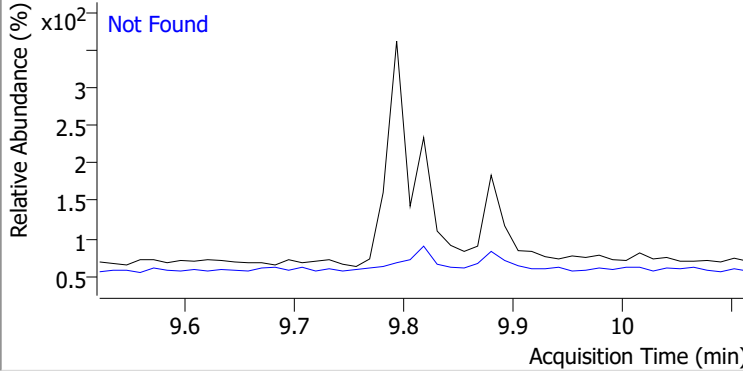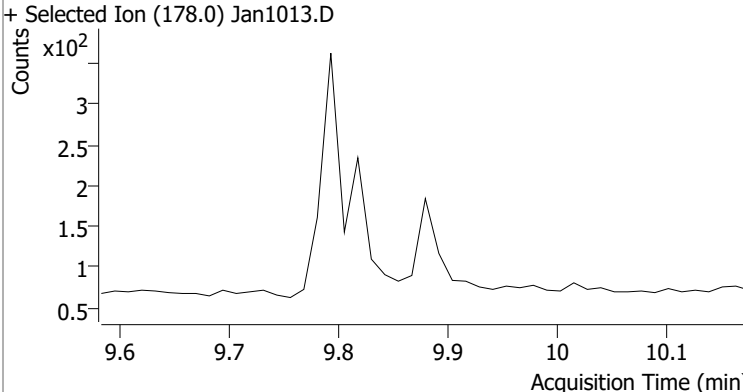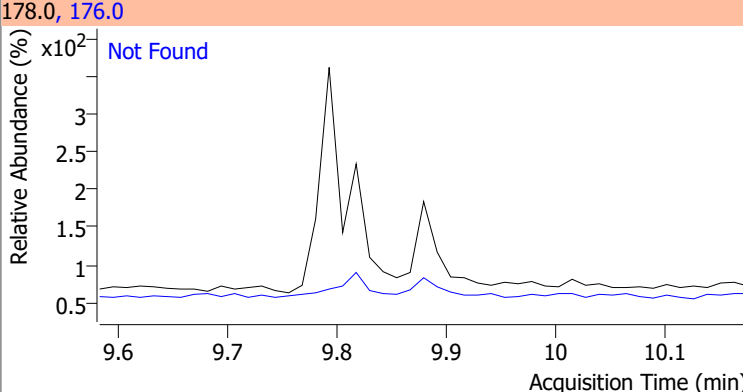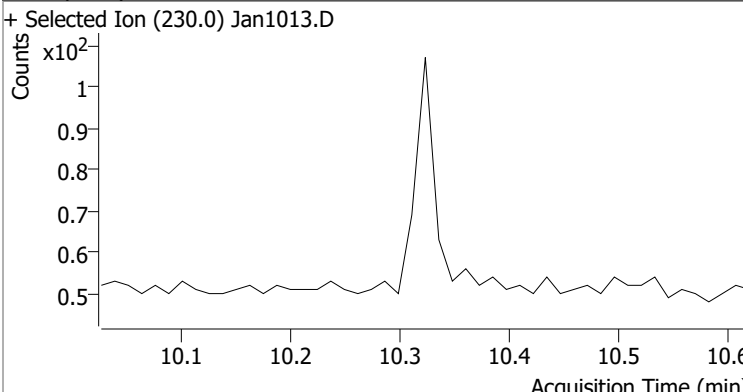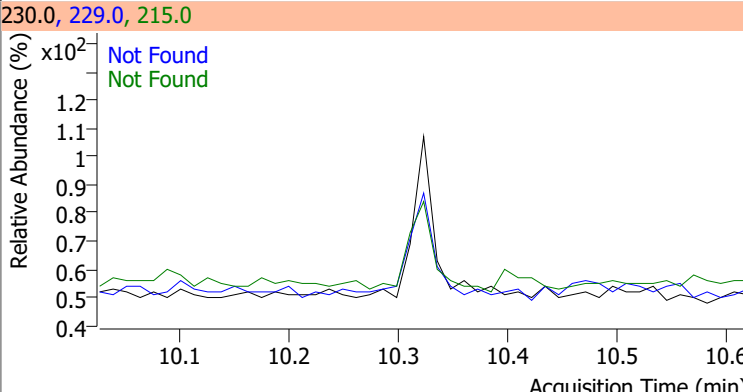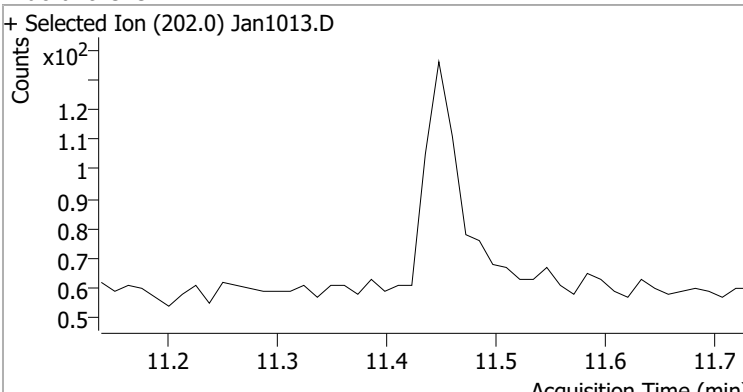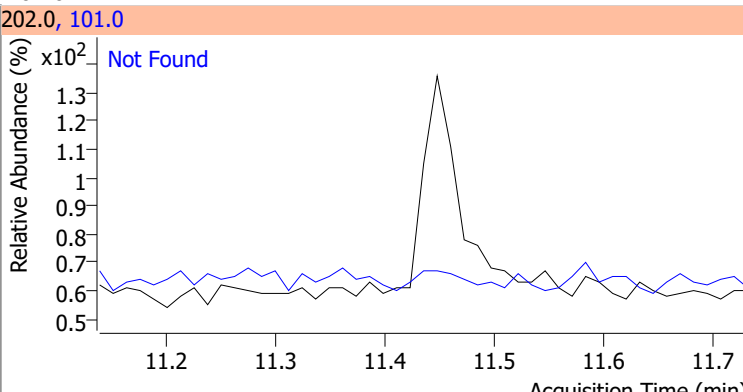
Compound	Conc.	Exp RT	QIon	Exp Ratio		
Phenanthrene	N.D.	9.82	176.0	15.5		
+ Selected Ion (178.0) Jan1013.D			178.0, 176.0			
						
Anthracene	N.D.	9.88	176.0	16.6		
+ Selected Ion (178.0) Jan1013.D			178.0, 176.0			
						
o-Terphenyl	N.D.	10.32	229.0	66.8	QIon	Exp Ratio
+ Selected Ion (230.0) Jan1013.D			230.0, 229.0, 215.0			
						
Fluoranthene	N.D.	11.44	101.0	11.4		
+ Selected Ion (202.0) Jan1013.D			202.0, 101.0			
						

Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.6	30.8




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1014.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/10/2022 6:12:08 PM
Sample Name	B21122105-001C	Instrument	GCMS
Vial	14	Multiplier	1.00
DA Method File	010522 bna SIM 3.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 1.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	237673	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	423270	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	253249	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.793	188.0	541953	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	409952	40.0000	ng/ml	-0.013
M Perylene-d12	18.524	264.0	287576	40.0000	ng/ml	0.000
System Monitoring Compounds						
S Nitrobenzene-d5	5.143	82.0	483480	42.6537	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 853.07%		*
S 2-Fluorobiphenyl	7.265	172.0	877617	69.6084	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1392.17%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.300	244.0	842979	111.1279	ng/ml	0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 2222.56%		*
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.013	154.0	0		ng/ml	md 1
T Fluorene	0.000		0	N.D.		
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.751	228.0	0		ng/ml	md 1
T Chrysene	14.751	228.0	0		ng/ml	md 1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.524	252.0	0		ng/ml md	1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	42.6537	5.14	-0.02	483480	54.0	34.4	21.6	40.2
					128.0	32.5	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4



Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio		
Phenanthrene	N.D.	9.82	176.0	15.5		
+ Selected Ion (178.0) Jan1014.D			178.0, 176.0			
Anthracene	N.D.	9.88	176.0	16.6		
+ Selected Ion (178.0) Jan1014.D			178.0, 176.0			
o-Terphenyl	N.D.	10.32	229.0	66.8	QIon	Exp Ratio
+ Selected Ion (230.0) Jan1014.D			230.0, 229.0, 215.0			
Fluoranthene	N.D.	11.44	101.0	11.4		
+ Selected Ion (202.0) Jan1014.D			202.0, 101.0			

Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Pyrene	N.D.	11.82	101.0	13.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	111.1279	12.30	0.01	842979	122.0	15.0	9.6	17.9



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)Anthracene	0	0	0	0	226.0		19.5	36.3
					229.0		16.5	30.6




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	0	0	0	0	226.0		22.2	41.2
					229.0		15.5	28.9




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.6	30.8




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1015.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/10/2022 6:44:28 PM
Sample Name	B21122105-001C	Instrument	GCMS
Vial	15	Multiplier	20.00
DA Method File	010522 bna SIM 3.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 1.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	219779	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	418524	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	263794	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.793	188.0	565970	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	435650	40.0000	ng/ml	-0.012
M Perylene-d12	18.524	264.0	322399	40.0000	ng/ml	0.000
System Monitoring Compounds						
S Nitrobenzene-d5	5.156	82.0	16728	63.4281	ng/ml	-0.012
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 1268.56%		*
S 2-Fluorobiphenyl	7.265	172.0	47193	71.8691	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1437.38%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.288	244.0	41710	103.4833	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 2069.67%		*
Target Compounds						QValue
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.050	154.0	0	ng/ml	md	1
T Fluorene	0.000		0	N.D.		
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	0.000		0	N.D.		
T Chrysene	14.751	228.0	0	ng/ml	md	1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.524	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	63.4281	5.16	-0.01	16728	54.0	30.9	21.6	40.2
					128.0	35.9	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	71.8691	7.26	0.00	47193	171.0	36.4	26.4	49.0




Compound	Conc.	Exp RT	QIon	Exp Ratio
Acenaphthylene	N.D.	7.84	153.0	14.6











Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene		0		0	153.0		80.3	149.2
					152.0		38.4	71.4



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Fluorene	N.D.	8.69	165.0	96.4	167.0	11.3




Quantitation Results Report (QT Reviewed)

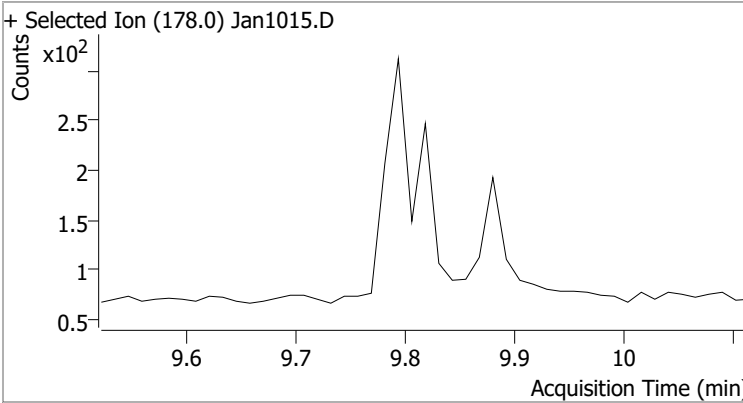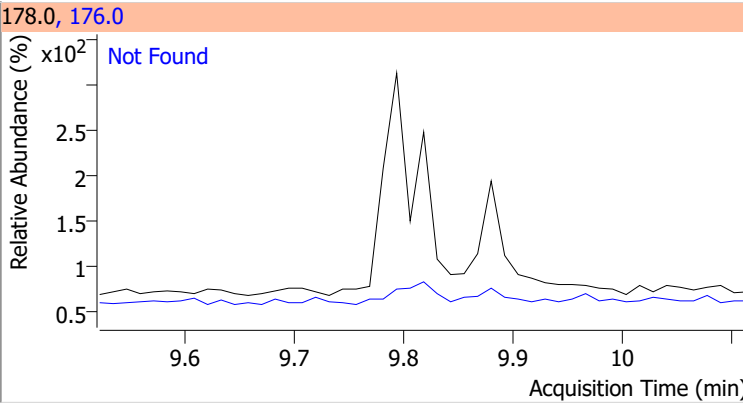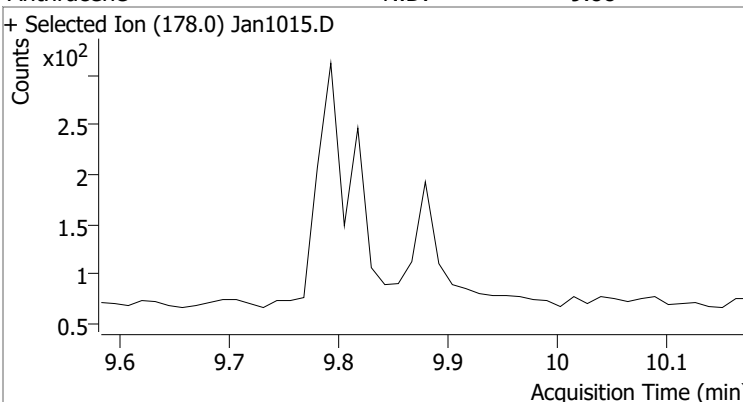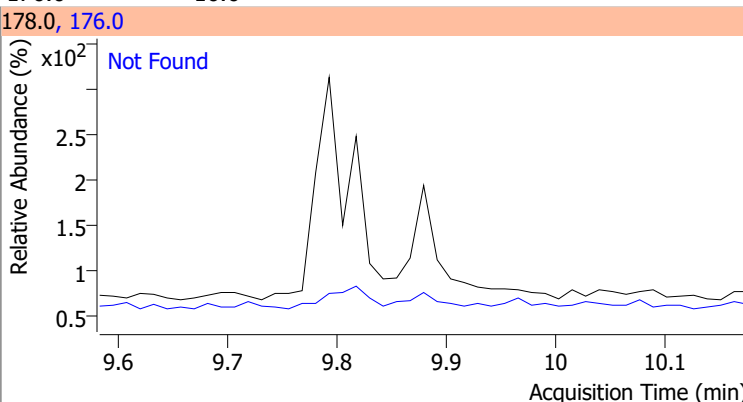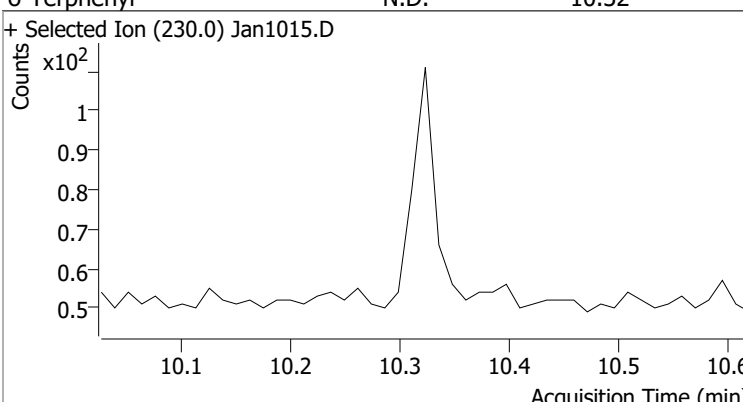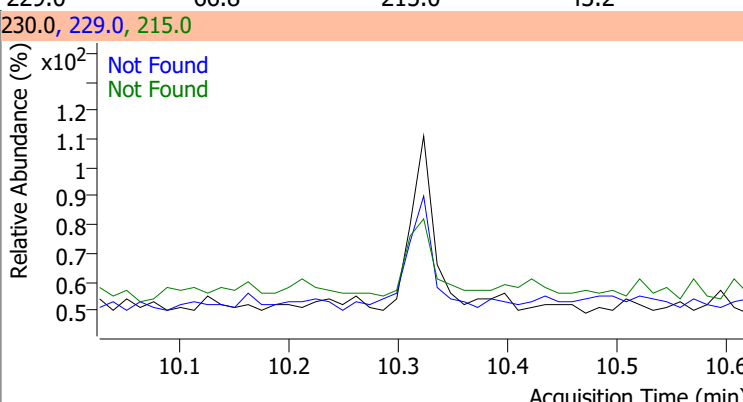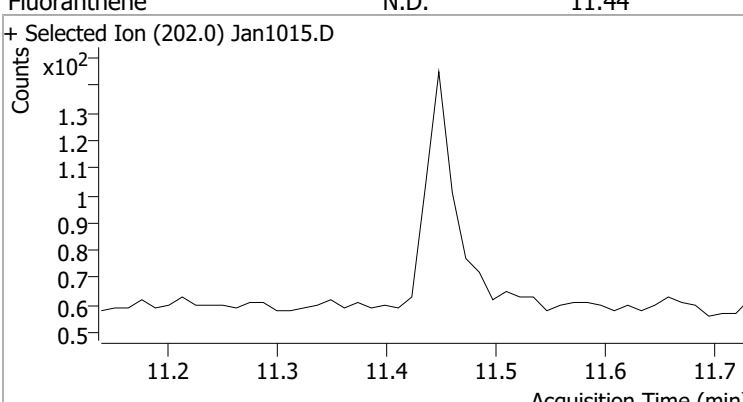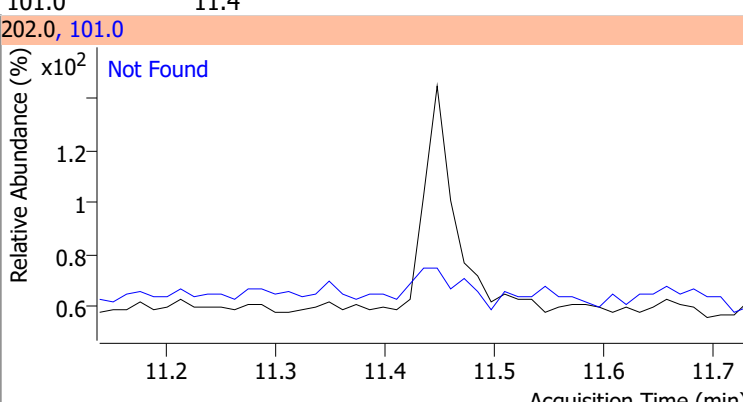
Compound	Conc.	Exp RT	QIon	Exp Ratio		
Phenanthrene	N.D.	9.82	176.0	15.5		
+ Selected Ion (178.0) Jan1015.D			178.0, 176.0			
						
Anthracene	N.D.	9.88	176.0	16.6		
+ Selected Ion (178.0) Jan1015.D			178.0, 176.0			
						
o-Terphenyl	N.D.	10.32	229.0	66.8	QIon	Exp Ratio
+ Selected Ion (230.0) Jan1015.D			230.0, 229.0, 215.0			
						
Fluoranthene	N.D.	11.44	101.0	11.4		
+ Selected Ion (202.0) Jan1015.D			202.0, 101.0			
						

Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Pyrene	N.D.	11.82	101.0	13.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	103.4833	12.29	0.00	41710	122.0	15.3	9.6	17.9



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(a)Anthracene	N.D.	14.73	226.0	27.9	229.0	23.5




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	0	0	0	0	226.0	22.2	15.5	41.2
					229.0	15.5	15.5	28.9




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.6	30.8




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1016.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/10/2022 7:16:52 PM
Sample Name	B21122105-001CLMS	Instrument	GCMS
Vial	16	Multiplier	1.00
DA Method File	010522 bna SIM 3.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 1.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	219113	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	400551	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	247615	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.793	188.0	548486	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	410476	40.0000	ng/ml	-0.013
M Perylene-d12	18.524	264.0	300428	40.0000	ng/ml	0.000
System Monitoring Compounds						
S Nitrobenzene-d5	5.156	82.0	16262	3.0985	ng/ml	-0.013
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 61.97%		
S 2-Fluorobiphenyl	7.264	172.0	48582	3.9410	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 78.82%		
S o-Terphenyl	10.324	230.0	43465	4.3219	ng/ml	0.000
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = 86.44%		
S Terphenyl-d14	12.288	244.0	38869	5.1175	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 102.35%		
Target Compounds						
T Naphthalene	5.966	128.0	44150	3.2825	ng/ml	100
T 2-Methylnaphthalene	6.790	141.0	27965	3.6052	ng/ml	97
T 1-Methylnaphthalene	6.902	141.0	27143	3.7844	ng/ml	95
T Acenaphthylene	7.838	152.0	52668	3.9772	ng/ml	100
T Acenaphthene	8.050	154.0	36030	3.7423	ng/ml	99
T Fluorene	8.673	166.0	49695	4.5106	ng/ml	98
T Phenanthrene	9.817	178.0	78286	4.7320	ng/ml	92
T Anthracene	9.879	178.0	69386	4.9863	ng/ml	95
T Fluoranthene	11.435	202.0	87304	4.6696	ng/ml	100
T Pyrene	11.806	202.0	95354	4.6567	ng/ml	98
T Benzo(a)Anthracene	14.726	228.0	62073	5.0122	ng/ml	99
T Chrysene	14.813	228.0	86043	5.0412	ng/ml	98
T Benzo(b)fluoranthene	17.746	252.0	57064	4.4054	ng/ml	98


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	17.807	252.0	62200	4.4906	ng/ml	99
T Benzo(a)pyrene	18.388	252.0	42537	4.3952	ng/ml	100
T Indeno(1,2,3-cd)pyrene	20.241	276.0	38658	4.2973	ng/ml	99
T Dibenzo(a,h)anthracene	20.316	278.0	49078	4.6961	ng/ml	98
T Benzo(g,h,i)perylene	20.575	276.0	63205	4.6213	ng/ml	99


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	3.0985	5.16	-0.01	16262	54.0	34.6	21.6	40.2
					128.0	35.1	21.3	39.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	3.2825	5.97	-0.01	44150	102.0	15.5	0.0	46.6
					129.0	11.1	7.6	14.1






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	3.6052	6.79	-0.01	27965	142.0	147.4	103.3	191.8
					115.0	61.6	36.8	68.3






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	3.7844	6.90	0.00	27143	142.0	116.6	77.9	144.7
					115.0	58.7	44.4	82.5






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	3.9410	7.26	0.00	48582	171.0	36.8	26.4	49.0















Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthylene	3.9772	7.84	0.00	52668	153.0	14.7	10.2	18.9



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	3.7423	8.05	0.00	36030	153.0	113.7	80.3	149.2
					152.0	54.0	38.4	71.4




Quantitation Results Report (QT Reviewed)

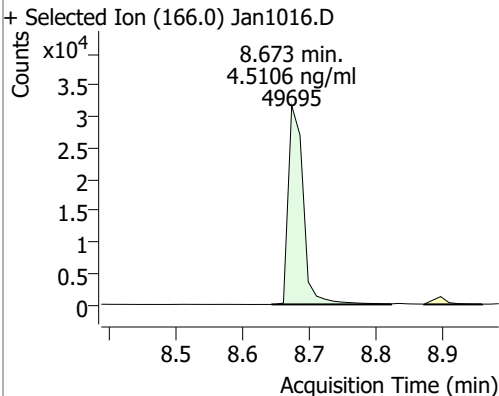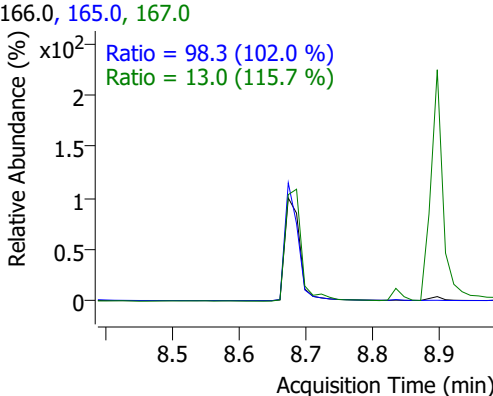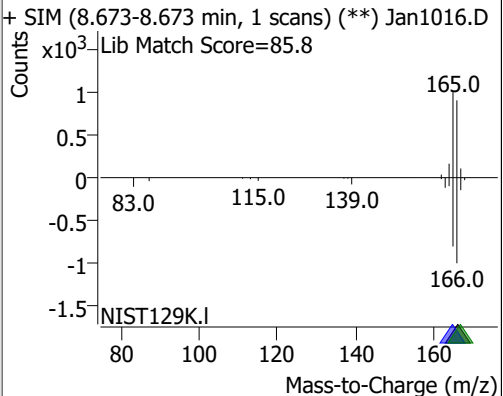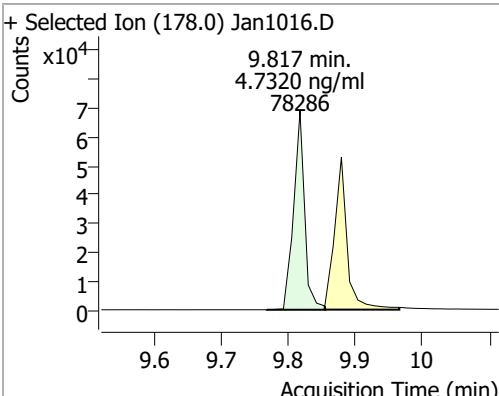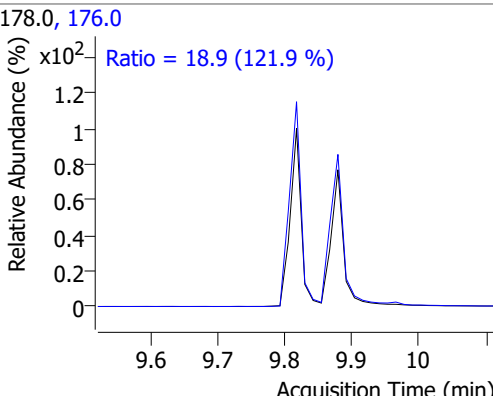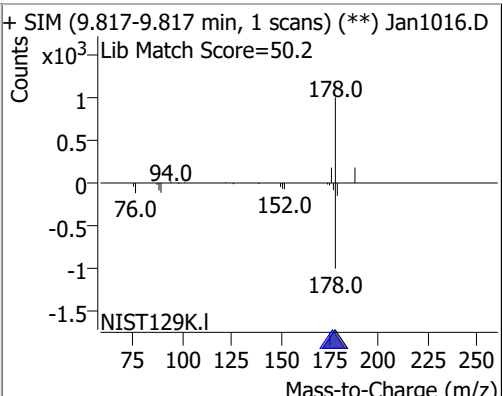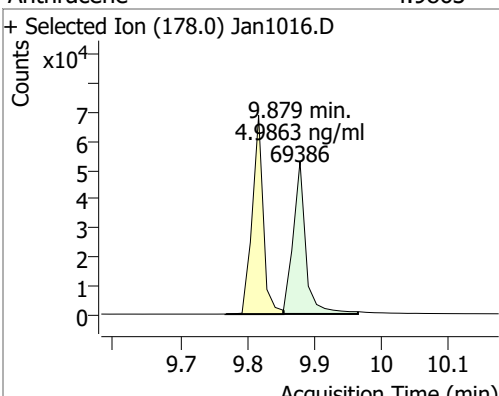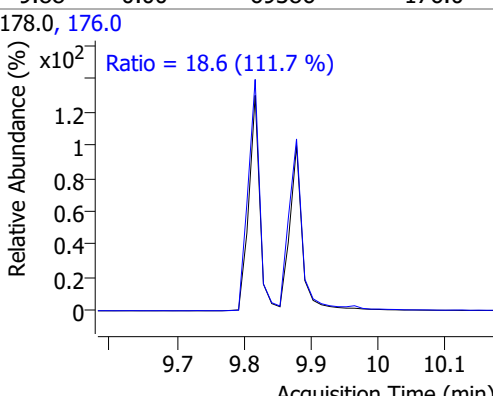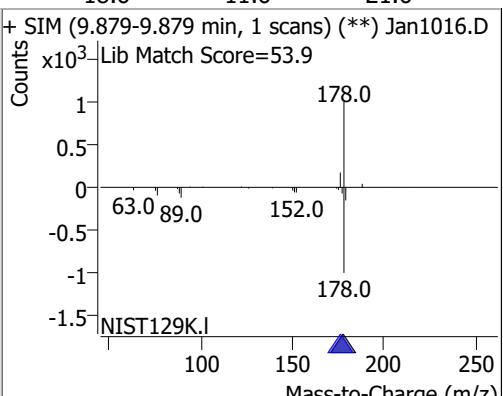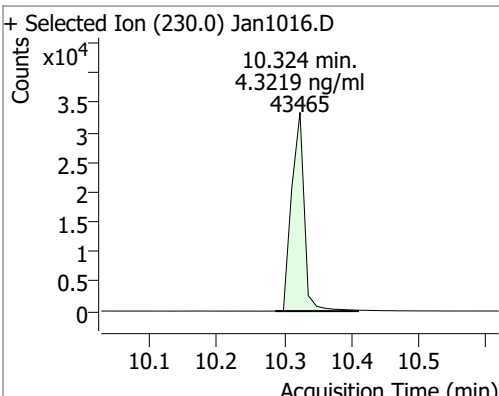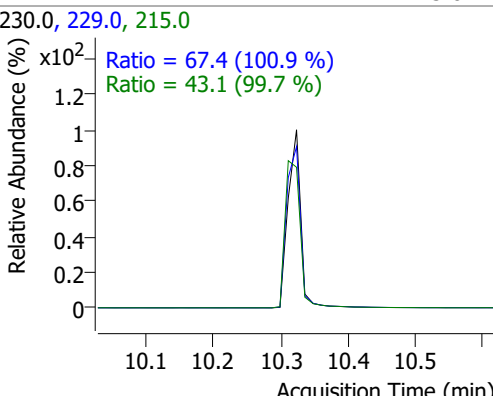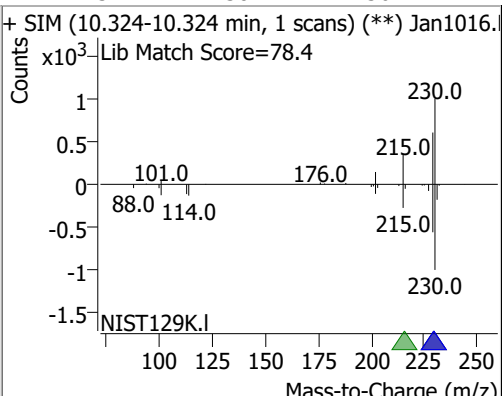
Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene	4.5106	8.67	-0.01	49695	165.0 167.0	98.3 13.0	67.5 7.9	125.3 14.6
+ Selected Ion (166.0) Jan1016.D 			166.0, 165.0, 167.0 			+ SIM (8.673-8.673 min, 1 scans) (**) Jan1016.D Lib Match Score=85.8 		
Phenanthrene	4.7320	9.82	0.00	78286	176.0	18.9	10.9	20.2
+ Selected Ion (178.0) Jan1016.D 			178.0, 176.0 			+ SIM (9.817-9.817 min, 1 scans) (**) Jan1016.D Lib Match Score=50.2 		
Anthracene	4.9863	9.88	0.00	69386	176.0	18.6	11.6	21.6
+ Selected Ion (178.0) Jan1016.D 			178.0, 176.0 			+ SIM (9.879-9.879 min, 1 scans) (**) Jan1016.D Lib Match Score=53.9 		
o-Terphenyl	4.3219	10.32	0.00	43465	229.0 215.0	67.4 43.1	46.7 30.2	86.8 56.2
+ Selected Ion (230.0) Jan1016.D 			230.0, 229.0, 215.0 			+ SIM (10.324-10.324 min, 1 scans) (**) Jan1016.D Lib Match Score=78.4 		

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluoranthene	4.6696	11.44	0.00	87304	101.0	11.3	8.0	14.8




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Pyrene	4.6567	11.81	-0.01	95354	101.0	13.2	9.7	18.1



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	5.1175	12.29	0.00	38869	122.0	14.7	9.6	17.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)Anthracene	5.0122	14.73	0.00	62073	226.0	27.7	19.5	36.3
					229.0	22.8	16.5	30.6




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	5.0412	14.81	-0.01	86043	226.0	30.5	22.2	41.2
					229.0	21.4	15.5	28.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(b)fluoranthene	4.4054	17.75	-0.01	57064	253.0	21.9	15.8	29.4



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(k)fluoranthene	4.4906	17.81	-0.01	62200	253.0	22.5	16.1	30.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene	4.3952	18.39	-0.01	42537	253.0	23.7	16.6	30.8




Quantitation Results Report (QT Reviewed)

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Indeno(1,2,3-cd)pyrene	4.2973	20.24	0.00	38658	138.0	24.5	17.6	32.7
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1016.D</p> </div> <div style="width: 30%;"> <p>276.0, 138.0</p> <p>Ratio = 24.5 (97.2 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.241-20.241 min, 1 scans) (**) Jan1016.D</p> <p>Lib Match Score=78.4</p> </div> </div>								
Dibenzo(a,h)anthracene	4.6961	20.32	0.00	49078	279.0	24.6	18.1	33.6
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (278.0) Jan1016.D</p> </div> <div style="width: 30%;"> <p>278.0, 279.0, 139.0</p> <p>Ratio = 24.6 (95.3 %)</p> <p>Ratio = 18.1 (99.2 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.316-20.316 min, 1 scans) (**) Jan1016.D</p> <p>Lib Match Score=77.2</p> </div> </div>								
Benzo(g,h,i)perylene	4.6213	20.58	0.00	63205	277.0	24.6	17.1	31.8
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1016.D</p> </div> <div style="width: 30%;"> <p>276.0, 138.0, 277.0</p> <p>Ratio = 20.6 (103.1 %)</p> <p>Ratio = 24.6 (100.4 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.575-20.575 min, 1 scans) (**) Jan1016.D</p> <p>Lib Match Score=78.4</p> </div> </div>								

Quantitation Results Report (QT Reviewed)

Data File	Jan1017.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/10/2022 7:49:10 PM
Sample Name	MB-162701	Instrument	GCMS
Vial	17	Multiplier	1.00
DA Method File	010522 bna SIM 3.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 1.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	226411	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	438999	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	257117	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.793	188.0	574682	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	433178	40.0000	ng/ml	-0.013
M Perylene-d12	18.524	264.0	314911	40.0000	ng/ml	0.000
System Monitoring Compounds						
S Nitrobenzene-d5	5.143	82.0	477803	43.6854	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 873.71%		*
S 2-Fluorobiphenyl	7.265	172.0	818529	63.9452	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1278.90%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.288	244.0	850079	106.0552	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 2121.10%		*
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.050	154.0	0		ng/ml	md 1
T Fluorene	0.000		0	N.D.		
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.751	228.0	0		ng/ml	md 1
T Chrysene	14.751	228.0	0		ng/ml	md 1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.524	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	43.6854	5.14	-0.02	477803	54.0	33.2	21.6	40.2
					128.0	31.9	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	63.9452	7.26	0.00	818529	171.0	39.4	26.4	49.0




Compound	Conc.	Exp RT	QIon	Exp Ratio
Acenaphthylene	N.D.	7.84	153.0	14.6











Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	0	0	0	0	153.0 152.0	80.3 38.4	149.2 71.4	



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Fluorene	N.D.	8.69	165.0	96.4	167.0	11.3




Quantitation Results Report (QT Reviewed)

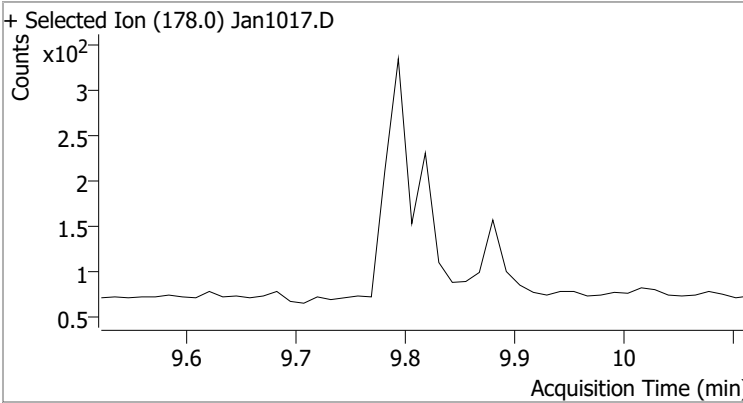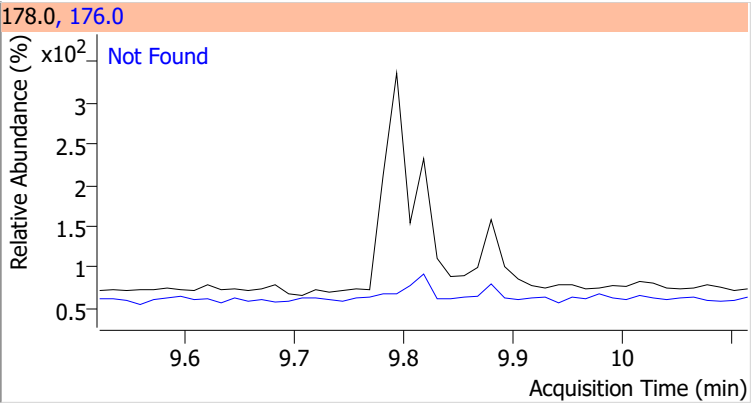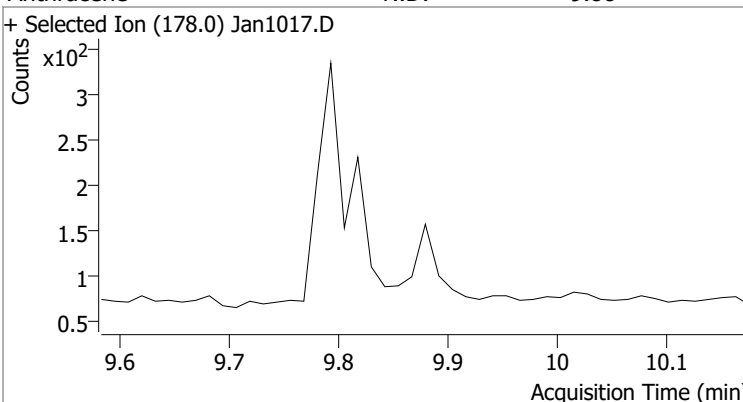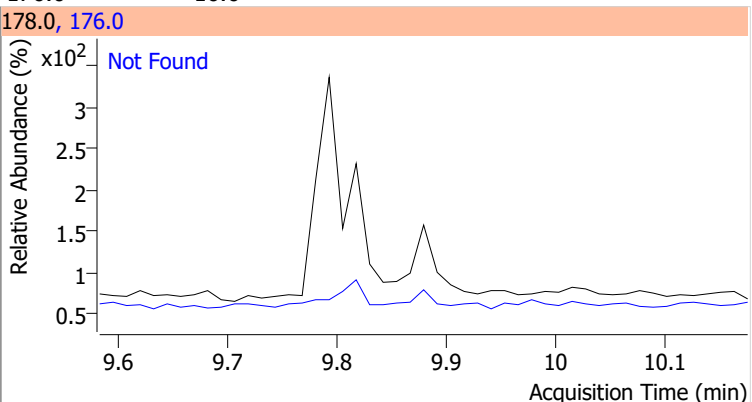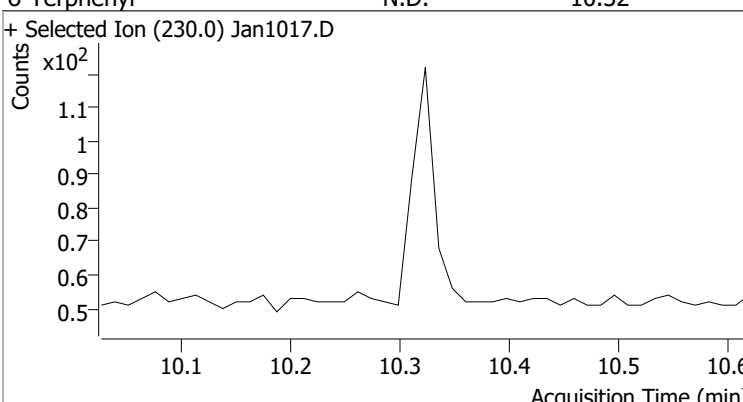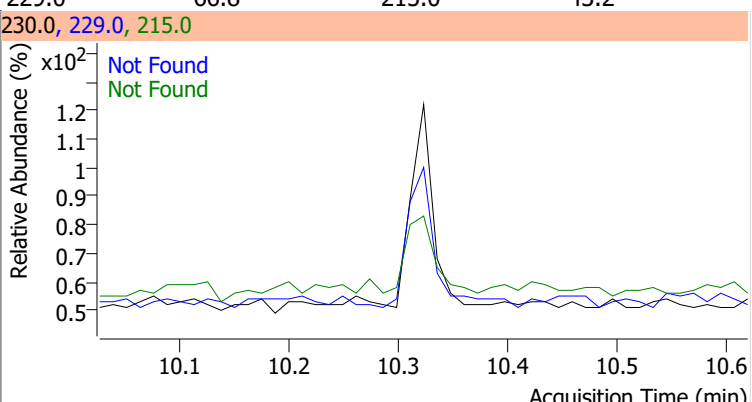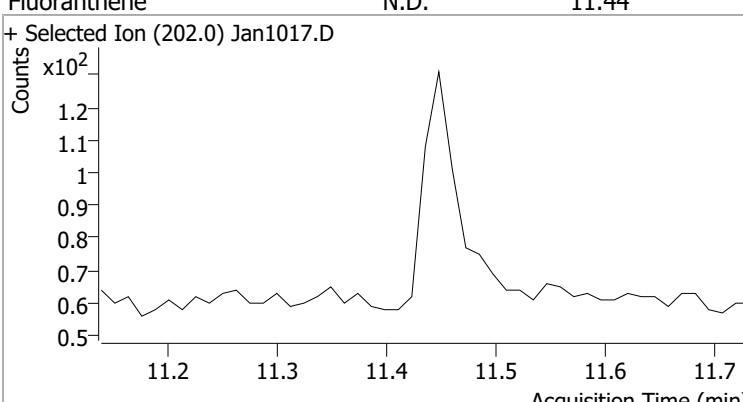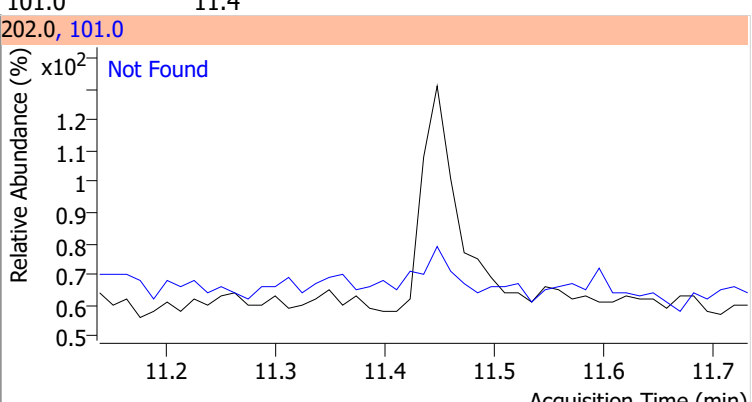
Compound	Conc.	Exp RT	QIon	Exp Ratio		
Phenanthrene	N.D.	9.82	176.0	15.5		
+ Selected Ion (178.0) Jan1017.D 			178.0, 176.0 			
Anthracene	N.D.	9.88	176.0	16.6		
+ Selected Ion (178.0) Jan1017.D 			178.0, 176.0 			
o-Terphenyl	N.D.	10.32	229.0	66.8	QIon	Exp Ratio
			215.0	43.2		
+ Selected Ion (230.0) Jan1017.D 			230.0, 229.0, 215.0 			
Fluoranthene	N.D.	11.44	101.0	11.4		
+ Selected Ion (202.0) Jan1017.D 			202.0, 101.0 			

Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Pyrene	N.D.	11.82	101.0	13.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	106.0552	12.29	0.00	850079	122.0	14.4	9.6	17.9



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)Anthracene		0		0	226.0 229.0		19.5 16.5	36.3 30.6




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene		0		0	226.0 229.0		22.2 15.5	41.2 28.9




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.6	30.8




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1018.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/10/2022 8:21:35 PM
Sample Name	MB-162701	Instrument	GCMS
Vial	18	Multiplier	20.00
DA Method File	010522 bna SIM 3.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 1.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	214295	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	409396	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	257702	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.793	188.0	560293	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	430415	40.0000	ng/ml	-0.013
M Perylene-d12	18.524	264.0	302731	40.0000	ng/ml	0.000
System Monitoring Compounds						
S Nitrobenzene-d5	5.156	82.0	16146	62.8368	ng/ml	-0.013
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 1256.74%		*
S 2-Fluorobiphenyl	7.264	172.0	41174	64.1852	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1283.70%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.288	244.0	38634	97.0182	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 1940.36%		*
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.050	154.0	0		ng/ml md	1
T Fluorene	0.000		0	N.D.		
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.751	228.0	0		ng/ml md	1
T Chrysene	14.751	228.0	0		ng/ml md	1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.524	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	62.8368	5.16	-0.01	16146	54.0	29.9	21.6	40.2
					128.0	34.1	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	64.1852	7.26	0.00	41174	171.0	35.7	26.4	49.0




Compound	Conc.	Exp RT	QIon	Exp Ratio
Acenaphthylene	N.D.	7.84	153.0	14.6











Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene		0		0	153.0		80.3	149.2
					152.0		38.4	71.4







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Fluorene	N.D.	8.69	165.0	96.4	167.0	11.3



Quantitation Results Report (QT Reviewed)

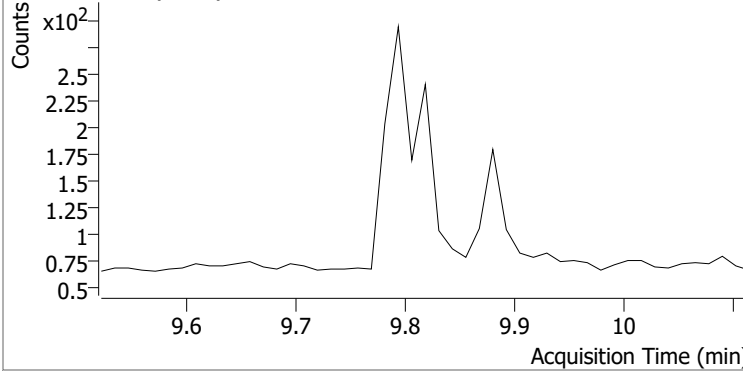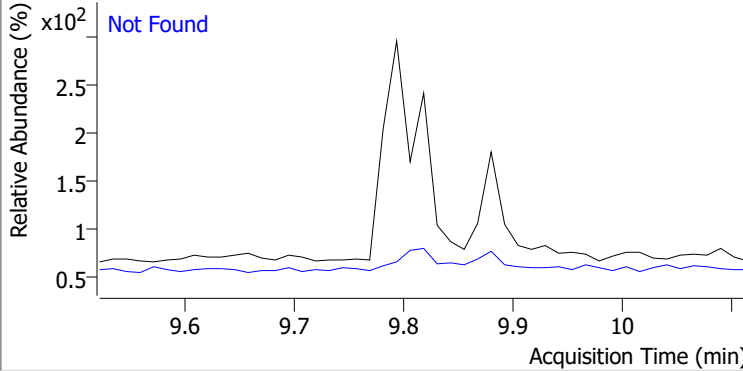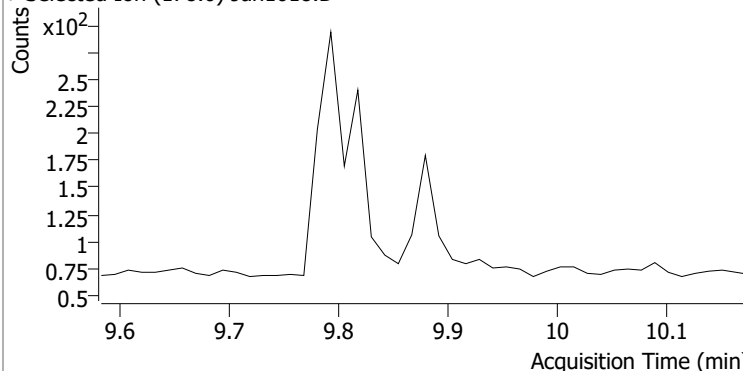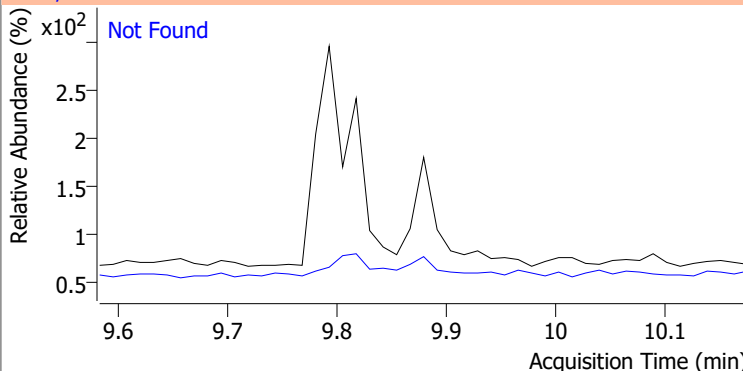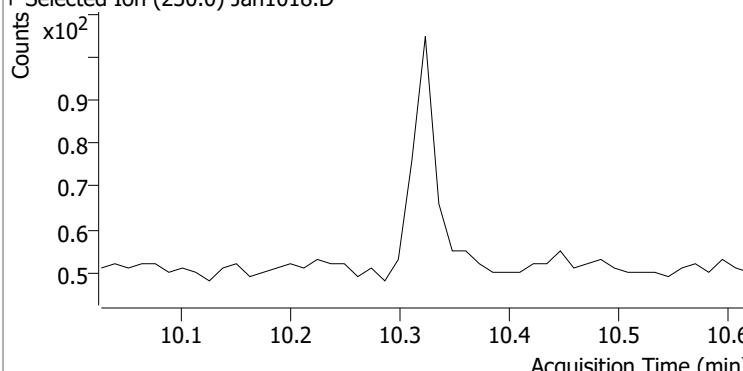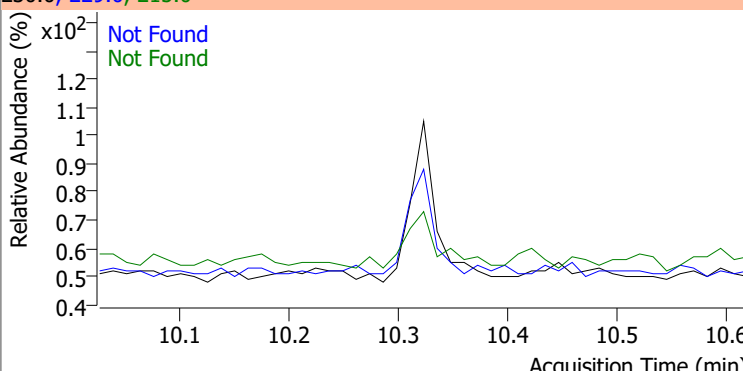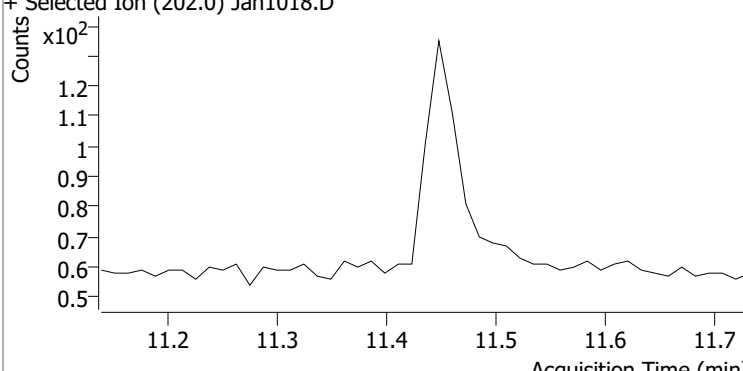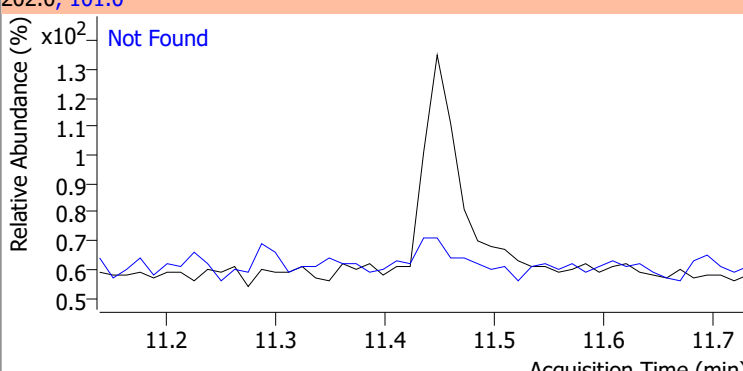
Compound	Conc.	Exp RT	QIon	Exp Ratio	
Phenanthrene	N.D.	9.82	176.0	15.5	
+ Selected Ion (178.0) Jan1018.D			178.0, 176.0		
				Not Found	
Anthracene	N.D.	9.88	176.0	16.6	
+ Selected Ion (178.0) Jan1018.D			178.0, 176.0		
				Not Found	
o-Terphenyl	N.D.	10.32	229.0	66.8	QIon: 215.0, Exp Ratio: 43.2
+ Selected Ion (230.0) Jan1018.D			230.0, 229.0, 215.0		
				Not Found	
Fluoranthene	N.D.	11.44	101.0	11.4	
+ Selected Ion (202.0) Jan1018.D			202.0, 101.0		
				Not Found	

Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.6	30.8




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1019.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/10/2022 8:53:55 PM
Sample Name	LLCS-162701	Instrument	GCMS
Vial	19	Multiplier	1.00
DA Method File	010522 bna SIM 3.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 1.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	229633	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	417162	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	253744	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.792	188.0	575427	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	439075	40.0000	ng/ml	-0.013
M Perylene-d12	18.524	264.0	315903	40.0000	ng/ml	0.000
System Monitoring Compounds						
S Nitrobenzene-d5	5.156	82.0	18854	3.4003	ng/ml	-0.013
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 68.01%		
S 2-Fluorobiphenyl	7.264	172.0	47296	3.7440	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 74.88%		
S o-Terphenyl	10.324	230.0	40680	3.8556	ng/ml	0.000
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = 77.11%		
S Terphenyl-d14	12.288	244.0	37432	4.6073	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 92.15%		
Target Compounds						
T Naphthalene	5.966	128.0	48239	3.4437	ng/ml	99
T 2-Methylnaphthalene	6.790	141.0	29239	3.6194	ng/ml	95
T 1-Methylnaphthalene	6.902	141.0	28578	3.8258	ng/ml	95
T Acenaphthylene	7.838	152.0	51185	3.7719	ng/ml	100
T Acenaphthene	8.050	154.0	35045	3.5521	ng/ml	100
T Fluorene	8.673	166.0	45946	4.0696	ng/ml	97
T Phenanthrene	9.817	178.0	72922	4.2022	ng/ml	92
T Anthracene	9.879	178.0	64717	4.4736	ng/ml	96
T Fluoranthene	11.435	202.0	78996	4.0274	ng/ml	99
T Pyrene	11.806	202.0	88177	4.0258	ng/ml	97
T Benzo(a)Anthracene	14.726	228.0	57805	4.3837	ng/ml	99
T Chrysene	14.813	228.0	81582	4.4835	ng/ml	98
T Benzo(b)fluoranthene	17.745	252.0	54922	4.0323	ng/ml	99


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	17.807	252.0	60206	4.1630	ng/ml	98
T Benzo(a)pyrene	18.388	252.0	40353	4.0093	ng/ml	100
T Indeno(1,2,3-cd)pyrene	20.241	276.0	38001	4.0173	ng/ml	98
T Dibenzo(a,h)anthracene	20.315	278.0	45963	4.1826	ng/ml	99
T Benzo(g,h,i)perylene	20.575	276.0	60406	4.2414	ng/ml	100


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	3.4003	5.16	-0.01	18854	54.0	35.8	21.6	40.2
					128.0	29.3	21.3	39.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	3.4437	5.97	-0.01	48239	102.0	15.0	0.0	46.6
					129.0	11.2	7.6	14.1




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	3.6194	6.79	-0.01	29239	142.0	144.6	103.3	191.8
					115.0	61.1	36.8	68.3




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	3.8258	6.90	0.00	28578	142.0	116.0	77.9	144.7
					115.0	58.0	44.4	82.5




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	3.7440	7.26	0.00	47296	171.0	36.1	26.4	49.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthylene	3.7719	7.84	0.00	51185	153.0	14.6	10.2	18.9






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	3.5521	8.05	0.00	35045	153.0	114.6	80.3	149.2
					152.0	55.3	38.4	71.4






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene	4.0696	8.67	-0.01	45946	165.0	98.9	67.5	125.3
					167.0	13.0	7.9	14.6






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Phenanthrene	4.2022	9.82	0.00	72922	176.0	18.9	10.9	20.2







Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Anthracene	4.4736	9.88	0.00	64717	176.0	18.4	11.6	21.6



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
o-Terphenyl	3.8556	10.32	0.00	40680	229.0	67.3	46.7	86.8
					215.0	42.7	30.2	56.2




Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	4.4835	14.81	-0.01	81582	226.0	30.4	22.2	41.2
					229.0	21.5	15.5	28.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(b)fluoranthene	4.0323	17.75	-0.01	54922	253.0	22.3	15.8	29.4



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(k)fluoranthene	4.1630	17.81	-0.01	60206	253.0	22.1	16.1	30.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene	4.0093	18.39	-0.01	40353	253.0	23.7	16.6	30.8




Quantitation Results Report (QT Reviewed)

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Indeno(1,2,3-cd)pyrene	4.0173	20.24	0.00	38001	138.0	23.9	17.6	32.7
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1019.D</p> </div> <div style="width: 30%;"> <p>276.0, 138.0</p> <p>Ratio = 23.9 (95.2 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.241-20.241 min, 1 scans) (**) Jan1019.D</p> <p>Lib Match Score=78.2</p> </div> </div>								
Dibenzo(a,h)anthracene	4.1826	20.32	0.00	45963	279.0	25.2	18.1	33.6
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (278.0) Jan1019.D</p> </div> <div style="width: 30%;"> <p>278.0, 279.0, 139.0</p> <p>Ratio = 25.2 (97.4 %)</p> <p>Ratio = 18.6 (101.5 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.315-20.315 min, 1 scans) (**) Jan1019.D</p> <p>Lib Match Score=76.7</p> </div> </div>								
Benzo(g,h,i)perylene	4.2414	20.57	0.00	60406	277.0	24.7	17.1	31.8
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1019.D</p> </div> <div style="width: 30%;"> <p>276.0, 138.0, 277.0</p> <p>Ratio = 20.0 (100.3 %)</p> <p>Ratio = 24.7 (100.7 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.575-20.575 min, 1 scans) (**) Jan1019.D</p> <p>Lib Match Score=78.2</p> </div> </div>								

Quantitation Results Report (QT Reviewed)

Data File	Jan1020.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/10/2022 9:26:22 PM
Sample Name	LLCSD-162701	Instrument	GCMS
Vial	20	Multiplier	1.00
DA Method File	010522 bna SIM 3.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 1.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	243904	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	455490	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	276867	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.793	188.0	615723	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	475374	40.0000	ng/ml	-0.013
M Perylene-d12	18.524	264.0	354296	40.0000	ng/ml	0.000
System Monitoring Compounds						
S Nitrobenzene-d5	5.156	82.0	17624	3.0228	ng/ml	# -0.013
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 60.46%		
S 2-Fluorobiphenyl	7.264	172.0	52419	3.8029	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 76.06%		
S o-Terphenyl	10.324	230.0	44103	3.9064	ng/ml	0.000
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = 78.13%		
S Terphenyl-d14	12.288	244.0	41431	4.7100	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 94.20%		
Target Compounds						
T Naphthalene	5.966	128.0	52659	3.4429	ng/ml	99
T 2-Methylnaphthalene	6.790	141.0	32593	3.6951	ng/ml	94
T 1-Methylnaphthalene	6.902	141.0	31680	3.8841	ng/ml	95
T Acenaphthylene	7.838	152.0	58654	3.9613	ng/ml	99
T Acenaphthene	8.050	154.0	40803	3.7903	ng/ml	98
T Fluorene	8.673	166.0	51072	4.1458	ng/ml	98
T Phenanthrene	9.817	178.0	78715	4.2391	ng/ml	91
T Anthracene	9.879	178.0	70392	4.5419	ng/ml	96
T Fluoranthene	11.435	202.0	89163	4.2482	ng/ml	99
T Pyrene	11.806	202.0	97807	4.1244	ng/ml	97
T Benzo(a)Anthracene	14.726	228.0	63935	4.4757	ng/ml	99
T Chrysene	14.814	228.0	88192	4.4769	ng/ml	98
T Benzo(b)fluoranthene	17.746	252.0	60050	3.9310	ng/ml	100


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	17.807	252.0	65445	4.0451	ng/ml	100
T Benzo(a)pyrene	18.388	252.0	44938	3.9839	ng/ml	98
T Indeno(1,2,3-cd)pyrene	20.241	276.0	42764	4.0310	ng/ml	98
T Dibenzo(a,h)anthracene	20.316	278.0	52374	4.2495	ng/ml	99
T Benzo(g,h,i)perylene	20.575	276.0	66292	4.1590	ng/ml	98


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	3.0228	5.16	-0.01	17624	54.0	45.4	21.6	40.2
					128.0	35.5	21.3	39.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	3.4429	5.97	-0.01	52659	102.0	15.7	0.0	46.6
					129.0	11.1	7.6	14.1




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	3.6951	6.79	-0.01	32593	142.0	142.7	103.3	191.8
					115.0	62.1	36.8	68.3




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	3.8841	6.90	0.00	31680	142.0	115.7	77.9	144.7
					115.0	59.4	44.4	82.5




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	3.8029	7.26	0.00	52419	171.0	36.9	26.4	49.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthylene	3.9613	7.84	0.00	58654	153.0	14.9	10.2	18.9






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	3.7903	8.05	0.00	40803	153.0	112.9	80.3	149.2
					152.0	53.7	38.4	71.4






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene	4.1458	8.67	-0.01	51072	165.0 167.0	98.2 13.3	67.5 7.9	125.3 14.6






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Phenanthrene	4.2391	9.82	0.00	78715	176.0	19.1	10.9	20.2



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Anthracene	4.5419	9.88	0.00	70392	176.0	18.5	11.6	21.6




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
o-Terphenyl	3.9064	10.32	0.00	44103	229.0 215.0	68.7 44.6	46.7 30.2	86.8 56.2




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
----------	-------	----	----------	-------	------	--------	-------	-------




Pyrene	4.1244	11.81	-0.01	97807	101.0	12.6	9.7	18.1
--------	--------	-------	-------	-------	-------	------	-----	------



Terphenyl-d14	4.7100	12.29	0.00	41431	122.0	14.7	9.6	17.9
---------------	--------	-------	------	-------	-------	------	-----	------




Benzo(a)Anthracene	4.4757	14.73	0.00	63935	226.0	27.9	19.5	36.3
					229.0	22.7	16.5	30.6




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	4.4769	14.81	-0.01	88192	226.0	30.5	22.2	41.2
					229.0	21.3	15.5	28.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(b)fluoranthene	3.9310	17.75	-0.01	60050	253.0	22.6	15.8	29.4



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(k)fluoranthene	4.0451	17.81	-0.01	65445	253.0	22.8	16.1	30.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene	3.9839	18.39	-0.01	44938	253.0	24.5	16.6	30.8




Quantitation Results Report (QT Reviewed)

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Indeno(1,2,3-cd)pyrene	4.0310	20.24	0.00	42764	138.0	24.0	17.6	32.7
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1020.D</p> </div> <div style="width: 30%;"> <p>276.0, 138.0</p> <p>Ratio = 24.0 (95.3 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.241-20.241 min, 1 scans) (**) Jan1020.D</p> <p>Lib Match Score=78.6</p> </div> </div>								
Dibenzo(a,h)anthracene	4.2495	20.32	0.00	52374	279.0	25.2	18.1	33.6
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (278.0) Jan1020.D</p> </div> <div style="width: 30%;"> <p>278.0, 279.0, 139.0</p> <p>Ratio = 25.2 (97.4 %)</p> <p>Ratio = 18.3 (100.3 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.316-20.316 min, 1 scans) (**) Jan1020.D</p> <p>Lib Match Score=77.3</p> </div> </div>								
Benzo(g,h,i)perylene	4.1590	20.58	0.00	66292	277.0	25.4	17.1	31.8
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1020.D</p> </div> <div style="width: 30%;"> <p>276.0, 138.0, 277.0</p> <p>Ratio = 20.8 (104.4 %)</p> <p>Ratio = 25.4 (103.9 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.575-20.575 min, 1 scans) (**) Jan1020.D</p> <p>Lib Match Score=78.6</p> </div> </div>								

Quantitation Results Report (QT Reviewed)

Data File	Jan1021.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/10/2022 9:58:38 PM
Sample Name	B22010096-001C	Instrument	GCMS
Vial	21	Multiplier	1.00
DA Method File	010522 bna SIM 3.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 1.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	238665	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	461193	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	279700	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.793	188.0	586928	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	467542	40.0000	ng/ml	-0.013
M Perylene-d12	18.524	264.0	338468	40.0000	ng/ml	0.000
System Monitoring Compounds						
S Nitrobenzene-d5	5.143	82.0	509903	44.0360	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 880.72%		*
S 2-Fluorobiphenyl	7.264	172.0	957326	68.7499	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1375.00%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.288	244.0	965591	111.6122	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 2232.24%		*
Target Compounds						
T Naphthalene	0.000		0	N.D.		QValue
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.013	154.0	0		ng/ml	md 1
T Fluorene	8.686	166.0	0		ng/ml	md 1
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.751	228.0	0		ng/ml	md 1
T Chrysene	14.751	228.0	0		ng/ml	md 1
T Benzo(b)fluoranthene	0.000		0	N.D.		




Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.512	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		



(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	44.0360	5.14	-0.03	509903	54.0	34.5	21.6	40.2
					128.0	31.6	21.3	39.5





Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	68.7499	7.26	0.00	957326	171.0	39.5	26.4	49.0




Compound	Conc.	Exp RT	QIon	Exp Ratio
Acenaphthylene	N.D.	7.84	153.0	14.6











Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	0	0	0	0	153.0 152.0	80.3 38.4	149.2 71.4	







Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene	0	0	0	0	165.0 167.0	67.5 7.9	125.3 14.6	



Quantitation Results Report (QT Reviewed)

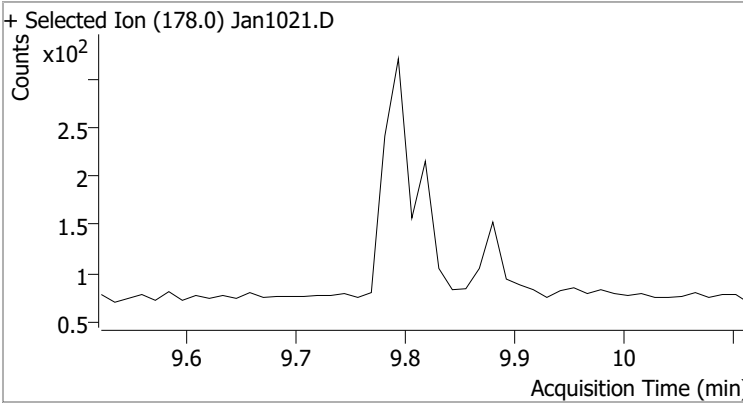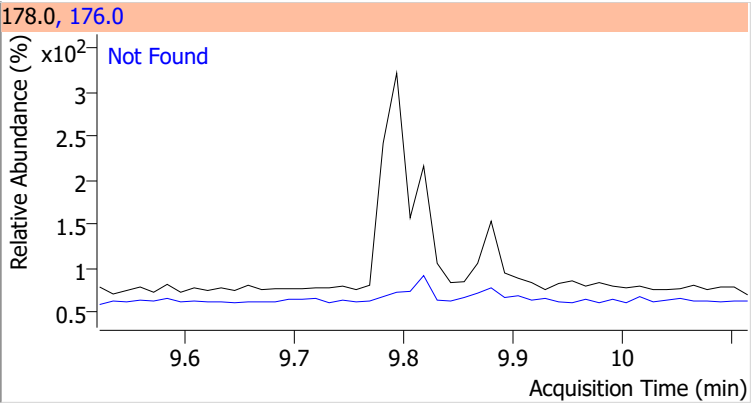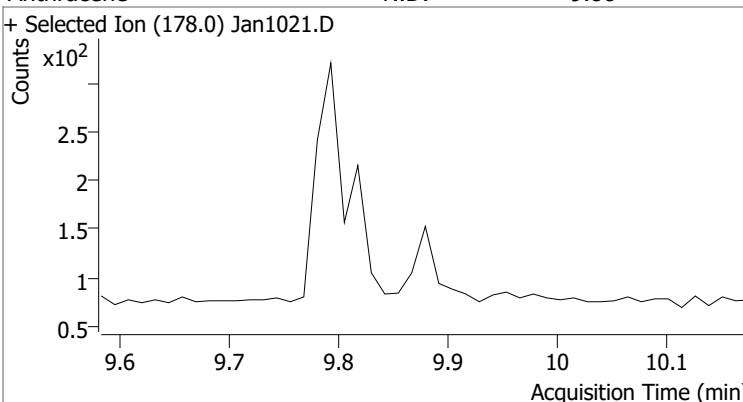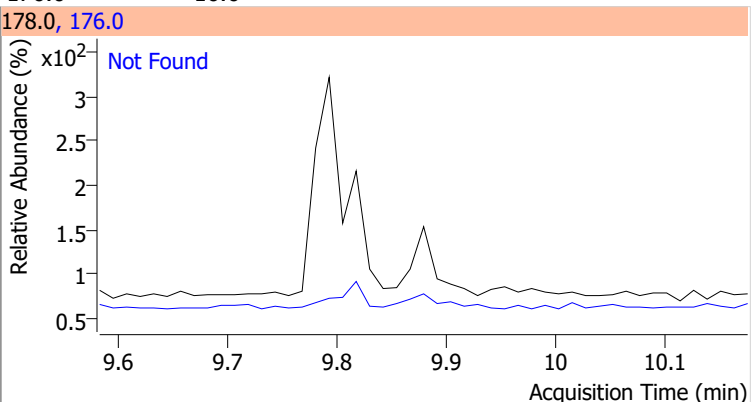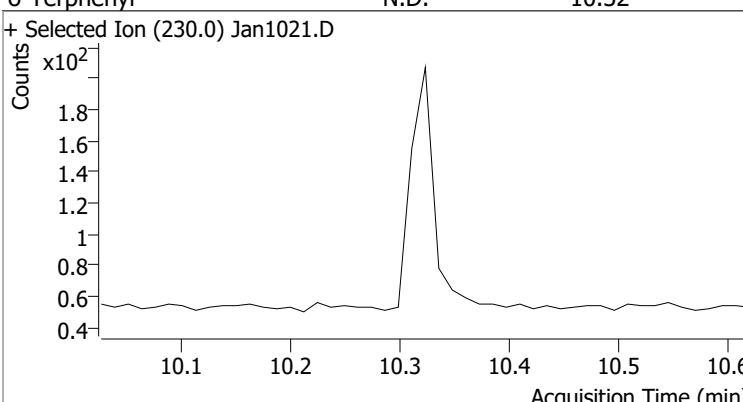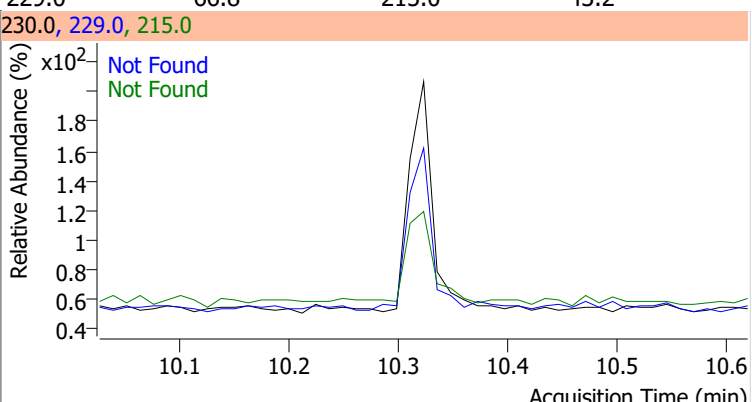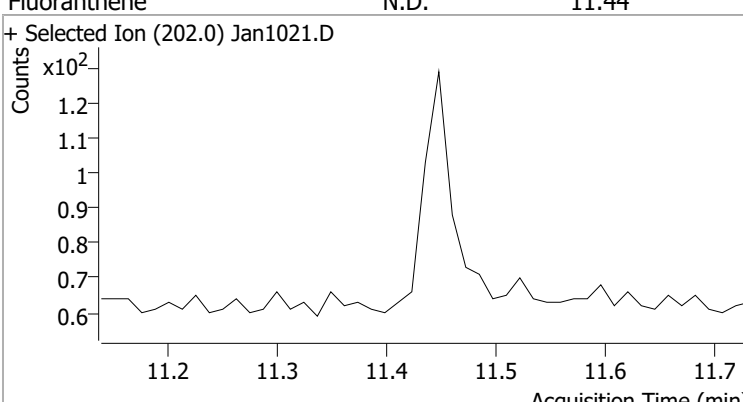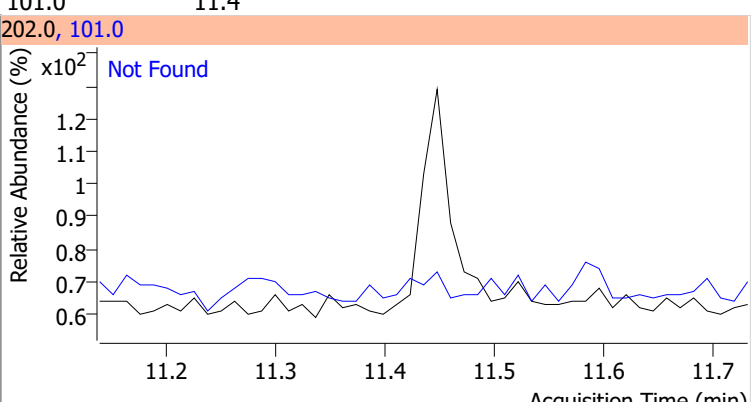
Compound	Conc.	Exp RT	QIon	Exp Ratio	
Phenanthrene	N.D.	9.82	176.0	15.5	
+ Selected Ion (178.0) Jan1021.D			178.0, 176.0		
					
Anthracene	N.D.	9.88	176.0	16.6	
+ Selected Ion (178.0) Jan1021.D			178.0, 176.0		
					
o-Terphenyl	N.D.	10.32	229.0	66.8	QIon: 215.0, Exp Ratio: 43.2
+ Selected Ion (230.0) Jan1021.D			230.0, 229.0, 215.0		
					
Fluoranthene	N.D.	11.44	101.0	11.4	
+ Selected Ion (202.0) Jan1021.D			202.0, 101.0		
					

Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.6	30.8




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1022.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/10/2022 10:31:04 PM
Sample Name	B22010096-001C	Instrument	GCMS
Vial	22	Multiplier	20.00
DA Method File	010522 bna SIM 3.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 1.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	232590	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	453174	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	270024	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.793	188.0	577465	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	468408	40.0000	ng/ml	-0.013
M Perylene-d12	18.524	264.0	340133	40.0000	ng/ml	0.000
System Monitoring Compounds						
S Nitrobenzene-d5	5.156	82.0	17926	64.1641	ng/ml	-0.013
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 1283.28% *		
S 2-Fluorobiphenyl	7.264	172.0	50605	75.2870	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1505.74% *		
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.288	244.0	46093	106.3605	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 2127.21% *		
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.050	154.0	0		ng/ml	md 1
T Fluorene	0.000		0	N.D.		
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.751	228.0	0		ng/ml	md 1
T Chrysene	14.751	228.0	0		ng/ml	md 1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.400	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	64.1641	5.16	-0.01	17926	54.0	33.1	21.6	40.2
					128.0	34.2	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5











Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4



Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)

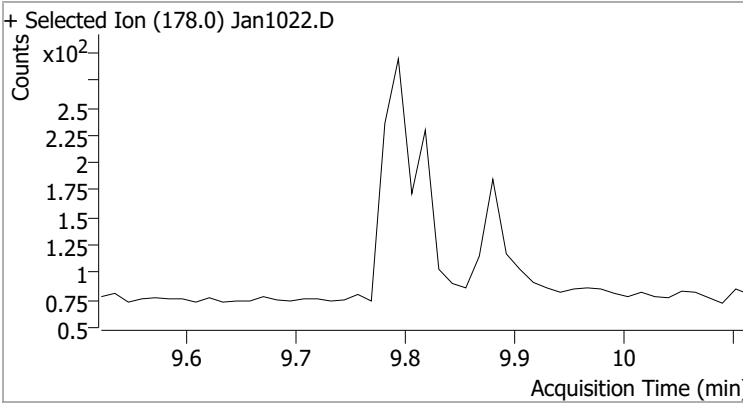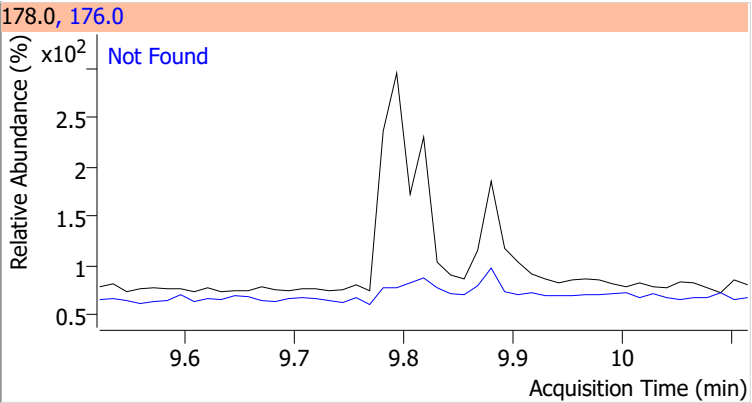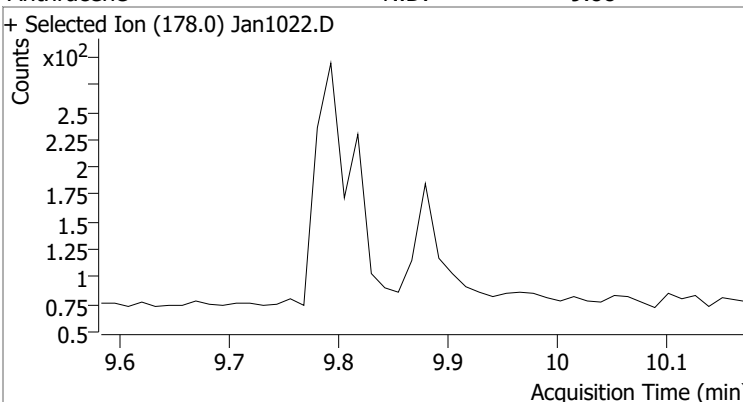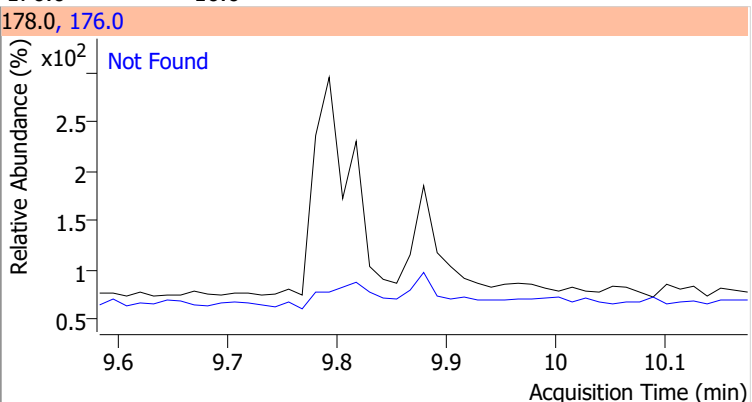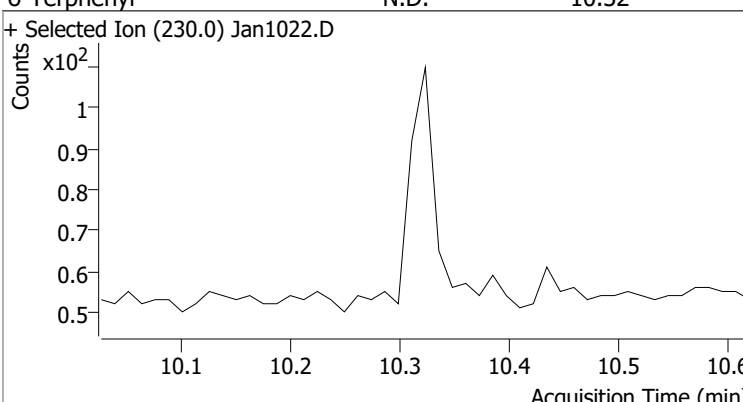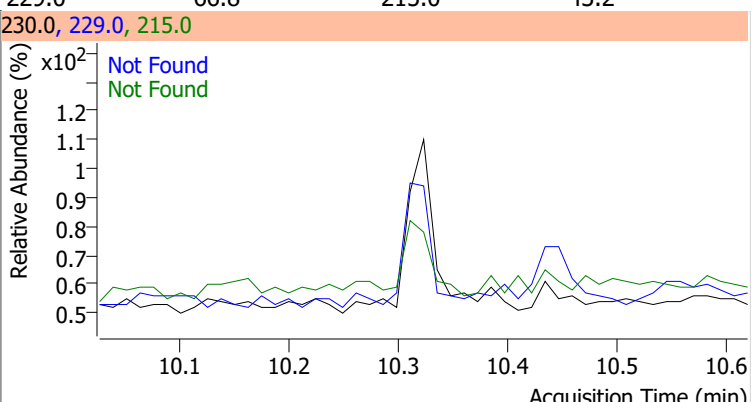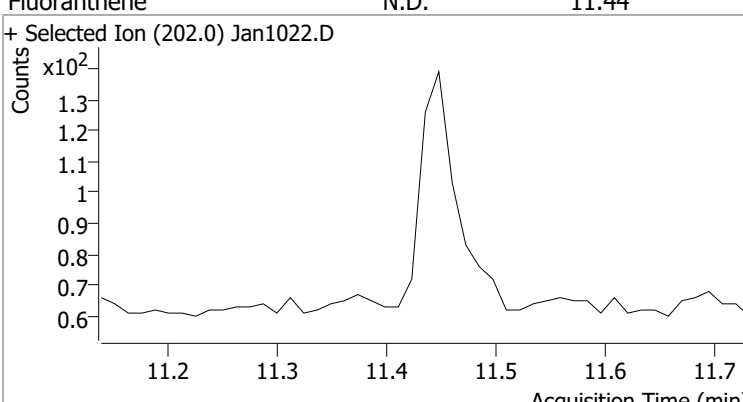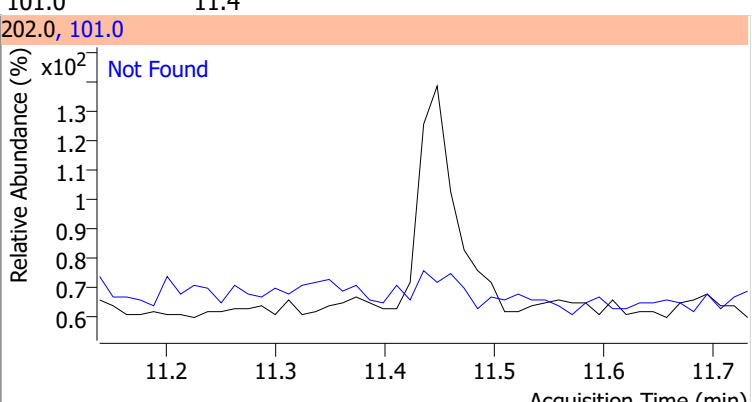
Compound	Conc.	Exp RT	QIon	Exp Ratio		
Phenanthrene	N.D.	9.82	176.0	15.5		
+ Selected Ion (178.0) Jan1022.D 			178.0, 176.0 			
Anthracene	N.D.	9.88	176.0	16.6		
+ Selected Ion (178.0) Jan1022.D 			178.0, 176.0 			
o-Terphenyl	N.D.	10.32	229.0	66.8	QIon	Exp Ratio
			215.0	43.2		
+ Selected Ion (230.0) Jan1022.D 			230.0, 229.0, 215.0 			
Fluoranthene	N.D.	11.44	101.0	11.4		
+ Selected Ion (202.0) Jan1022.D 			202.0, 101.0 			

Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Pyrene	N.D.	11.82	101.0	13.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	106.3605	12.29	0.00	46093	122.0	15.0	9.6	17.9



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)Anthracene		0		0	226.0		19.5	36.3
					229.0		16.5	30.6




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene		0		0	226.0		22.2	41.2
					229.0		15.5	28.9




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.6	30.8




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1023.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/10/2022 11:03:34 PM
Sample Name	10-Jan-22_CCV_23	Instrument	GCMS
Vial	23	Multiplier	1.00
DA Method File	010522 bna SIM 3.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 1.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	217229	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	420260	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	262061	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.792	188.0	542701	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	423306	40.0000	ng/ml	-0.013
M Perylene-d12	18.524	264.0	303138	40.0000	ng/ml	0.000
System Monitoring Compounds						
S Nitrobenzene-d5	5.155	82.0	8393	1.6811	ng/ml	-0.013
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 33.62%		
S 2-Fluorobiphenyl	7.264	172.0	24496	1.8776	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 37.55%		
S o-Terphenyl	10.324	230.0	17311	1.7396	ng/ml	0.000
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = 34.79%		*
S Terphenyl-d14	12.288	244.0	15641	1.9968	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 39.94%		
Target Compounds						
T Naphthalene	5.965	128.0	26295	1.8633	ng/ml	99
T 2-Methylnaphthalene	6.790	141.0	15984	1.9640	ng/ml	90
T 1-Methylnaphthalene	6.902	141.0	16773	2.2289	ng/ml	92
T Acenaphthylene	7.838	152.0	25307	1.8057	ng/ml	99
T Acenaphthene	8.050	154.0	16626	1.6317	ng/ml	99
T Fluorene	8.673	166.0	22351	1.9169	ng/ml	98
T Phenanthrene	9.817	178.0	31947	1.9385	ng/ml	91
T Anthracene	9.879	178.0	25997	1.9757	ng/ml	95
T Fluoranthene	11.435	202.0	33781	1.8261	ng/ml	99
T Pyrene	11.806	202.0	37773	1.7888	ng/ml	99
T Benzo(a)Anthracene	14.714	228.0	24230	1.8836	ng/ml	99
T Chrysene	14.813	228.0	33642	1.9333	ng/ml	99
T Benzo(b)fluoranthene	17.745	252.0	21409	1.6380	ng/ml	100


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	17.820	252.0	24566	1.8468	ng/ml	96
T Benzo(a)pyrene	18.400	252.0	16513	1.8124	ng/ml	99
T Indeno(1,2,3-cd)pyrene	20.254	276.0	15056	1.6587	ng/ml	95
T Dibenzo(a,h)anthracene	20.315	278.0	18550	1.7591	ng/ml	98
T Benzo(g,h,i)perylene	20.575	276.0	23331	1.8077	ng/ml	95


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	1.6811	5.16	-0.01	8393	54.0	36.9	21.6	40.2
					128.0	34.5	21.3	39.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	1.8633	5.97	-0.01	26295	102.0	15.1	0.0	46.6
					129.0	10.9	7.6	14.1




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	1.9640	6.79	-0.01	15984	142.0	136.0	103.3	191.8
					115.0	60.4	36.8	68.3




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	2.2289	6.90	0.00	16773	142.0	118.2	77.9	144.7
					115.0	55.6	44.4	82.5




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	1.8776	7.26	0.00	24496	171.0	36.2	26.4	49.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthylene	1.8057	7.84	0.00	25307	153.0	15.2	10.2	18.9






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	1.6317	8.05	0.00	16626	153.0	113.5	80.3	149.2
					152.0	53.5	38.4	71.4






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene	1.9169	8.67	-0.01	22351	165.0	98.1	67.5	125.3
					167.0	12.9	7.9	14.6






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Phenanthrene	1.9385	9.82	0.00	31947	176.0	19.5	10.9	20.2







Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Anthracene	1.9757	9.88	0.00	25997	176.0	18.9	11.6	21.6



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
o-Terphenyl	1.7396	10.32	0.00	17311	229.0	68.1	46.7	86.8
					215.0	43.7	30.2	56.2




Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	1.9333	14.81	-0.01	33642	226.0	30.9	22.2	41.2
					229.0	21.9	15.5	28.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(b)fluoranthene	1.6380	17.75	-0.01	21409	253.0	22.5	15.8	29.4



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(k)fluoranthene	1.8468	17.82	0.00	24566	253.0	24.9	16.1	30.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene	1.8124	18.40	0.00	16513	253.0	24.4	16.6	30.8



Quantitation Results Report (QT Reviewed)

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Indeno(1,2,3-cd)pyrene	1.6587	20.25	0.01	15056	138.0	27.6	17.6	32.7
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1023.D</p> </div> <div style="width: 30%;"> <p>276.0, 138.0</p> <p>Ratio = 27.6 (109.7 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.254-20.254 min, 1 scans) (**) Jan1023.D</p> <p>Lib Match Score=75.8</p> </div> </div>								
Dibenzo(a,h)anthracene	1.7591	20.32	0.00	18550	279.0	24.9	18.1	33.6
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (278.0) Jan1023.D</p> </div> <div style="width: 30%;"> <p>278.0, 279.0, 139.0</p> <p>Ratio = 24.9 (96.3 %)</p> <p>Ratio = 19.3 (105.6 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.315-20.315 min, 1 scans) (**) Jan1023.D</p> <p>Lib Match Score=75.4</p> </div> </div>								
Benzo(g,h,i)perylene	1.8077	20.57	0.00	23331	277.0	27.1	17.1	31.8
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1023.D</p> </div> <div style="width: 30%;"> <p>276.0, 138.0, 277.0</p> <p>Ratio = 22.5 (112.5 %)</p> <p>Ratio = 27.1 (110.8 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.575-20.575 min, 1 scans) (**) Jan1023.D</p> <p>Lib Match Score=75.9</p> </div> </div>								

Continuing Calibration Report

Batch Name \\MASSHUNTER\Org\Data\SV5975.I\sh011022\1 e8270d bna SIM\QuantResults\011022 bna SIM 1.batch.bin
Method File \\MASSHUNTER\Org\Data\SV5975.I\sh010522\3 e8270d bna SIM\010522 bna SIM 3.batch.bin
Daily CC \\MASSHUNTER\Org\Data\SV5975.I\sh011022\1 e8270d bna SIM\Jan1002.D

Level name	Injection Time	Calibration Files
7	12/28/2021 5:30:40 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2802.D
6	12/28/2021 6:03:21 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2803.D
5	12/28/2021 6:35:53 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2804.D
4	12/28/2021 7:08:33 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2805.D
3	12/28/2021 7:41:06 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2806.D
2	12/28/2021 8:13:46 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2807.D
1	12/28/2021 8:46:23 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2808.D
CCV	1/10/2022 11:43:19 AM	\\MASSHUNTER\Org\Data\SV5975.I\sh011022\1 e8270d bna SIM\Jan1002.D <=====

ISTD Compound:	Avg Resp	Mid Resp	CC Resp	Area%	A/M
1,4-Dichlorobenzene-d4	305106	324694	254870	78.50	M
Naphthalene-d8	572584	593232	433340	73.05	M
Acenaphthene-d10	319385	333337	258334	77.50	M
Phenanthrene-d10	689765	735690	564864	76.78	M
Chrysene-d12	520451	540068	417462	77.30	M
Perylene-d12	336551	351697	283136	80.51	M

Target Compound	AvgRF/R2	CC RF	Exp. Conc	Calc. Conc	%Dev	Area%	Curve Fit
1,4-Dichlorobenzene-d4	-----ISTD-----						
Nitrobenzene-d5	0.9996	0.7841	2.00	1.70	14.77	69.18	Quadratic
Naphthalene-d8	-----ISTD-----						
Naphthalene	1.3431	1.2782	2.00	1.90	-4.84	73.05	Avg RF
2-Methylnaphthalene	0.7746	0.7256	2.00	1.87	-6.32	73.06	Avg RF
1-Methylnaphthalene	0.7163	0.7727	2.00	2.16	7.88	85.81	Avg RF
Acenaphthene-d10	-----ISTD-----						
2-Fluorobiphenyl	1.9914	1.9185	2.00	1.93	-3.66	82.48	Avg RF
Acenaphthylene	2.1392	2.1102	2.00	1.97	-1.36	84.93	Avg RF
Acenaphthene	1.5553	1.4064	2.00	1.81	-9.57	75.26	Avg RF
Fluorene	1.7797	1.6959	2.00	1.91	-4.71	79.82	Avg RF
Phenanthrene-d10	-----ISTD-----						
Phenanthrene	0.9990	1.1492	2.00	1.89	5.44	75.85	Quadratic
Anthracene	0.9997	0.9979	2.00	2.06	-2.83	80.44	Quadratic
o-Terphenyl	0.7334	0.6543	2.00	1.78	-10.80	78.17	Avg RF
Fluoranthene	1.3635	1.2383	2.00	1.82	-9.18	78.10	Avg RF
Chrysene-d12	-----ISTD-----						
Pyrene	1.9954	1.8320	2.00	1.84	-8.19	77.86	Avg RF
Terphenyl-d14	0.7402	0.7260	2.00	1.96	-1.91	82.46	Avg RF
Benzo(a)Anthracene	0.9978	1.0912	2.00	1.79	10.50	71.35	Quadratic
Chrysene	0.9966	1.6085	2.00	1.96	2.17	77.50	Quadratic
Perylene-d12	-----ISTD-----						
Benzo(b)fluoranthene	1.7246	1.3886	2.00	1.61	-19.49	67.27	Avg RF
Benzo(k)fluoranthene	0.9999	1.6199	2.00	1.85	7.71	72.36	Quadratic
Benzo(a)pyrene	0.9996	1.1224	2.00	1.87	6.75	74.86	Quadratic
Indeno(1,2,3-cd)pyrene	1.1977	1.0048	2.00	1.68	-16.11	73.64	Avg RF
Dibenzo(a,h)anthracene	1.3915	1.2335	2.00	1.77	-11.36	76.99	Avg RF
Benzo(g,h,i)perylene	0.9993	1.4791	2.00	1.74	13.05	68.74	Quadratic

A -- against Average; M -- against Mid Point; P -- against Previous CC in the Method;

Continuing Calibration Report

Batch Name \\MASSHUNTER\Org\Data\SV5975.I\sh011022\1 e8270d bna SIM\QuantResults\011022 bna SIM 1.batch.bin
Method File \\MASSHUNTER\Org\Data\SV5975.I\sh010522\3 e8270d bna SIM\010522 bna SIM 3.batch.bin
Daily CC \\MASSHUNTER\Org\Data\SV5975.I\sh011022\1 e8270d bna SIM\Jan1023.D

Level name	Injection Time	Calibration Files
7	12/28/2021 5:30:40 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2802.D
6	12/28/2021 6:03:21 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2803.D
5	12/28/2021 6:35:53 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2804.D
4	12/28/2021 7:08:33 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2805.D
3	12/28/2021 7:41:06 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2806.D
2	12/28/2021 8:13:46 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2807.D
1	12/28/2021 8:46:23 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2808.D
CCV	1/10/2022 11:03:34 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh011022\1 e8270d bna SIM\Jan1023.D <=====

ISTD Compound:	Avg Resp	Mid Resp	CC Resp	Area%	A/M
1,4-Dichlorobenzene-d4	305106	324694	254870	78.50	M
Naphthalene-d8	572584	593232	433340	73.05	M
Acenaphthene-d10	319385	333337	258334	77.50	M
Phenanthrene-d10	689765	735690	564864	76.78	M
Chrysene-d12	520451	540068	417462	77.30	M
Perylene-d12	336551	351697	283136	80.51	M

Target Compound	AvgRF/R2	CC RF	Exp. Conc	Calc. Conc	%Dev	Area%	Curve Fit
1,4-Dichlorobenzene-d4	-----ISTD-----						
Nitrobenzene-d5	0.9996	0.7841	2.00	1.70	14.77	69.18	Quadratic
Naphthalene-d8	-----ISTD-----						
Naphthalene	1.3431	1.2782	2.00	1.90	-4.84	73.05	Avg RF
2-Methylnaphthalene	0.7746	0.7256	2.00	1.87	-6.32	73.06	Avg RF
1-Methylnaphthalene	0.7163	0.7727	2.00	2.16	7.88	85.81	Avg RF
Acenaphthene-d10	-----ISTD-----						
2-Fluorobiphenyl	1.9914	1.9185	2.00	1.93	-3.66	82.48	Avg RF
Acenaphthylene	2.1392	2.1102	2.00	1.97	-1.36	84.93	Avg RF
Acenaphthene	1.5553	1.4064	2.00	1.81	-9.57	75.26	Avg RF
Fluorene	1.7797	1.6959	2.00	1.91	-4.71	79.82	Avg RF
Phenanthrene-d10	-----ISTD-----						
Phenanthrene	0.9990	1.1492	2.00	1.89	5.44	75.85	Quadratic
Anthracene	0.9997	0.9979	2.00	2.06	-2.83	80.44	Quadratic
o-Terphenyl	0.7334	0.6543	2.00	1.78	-10.80	78.17	Avg RF
Fluoranthene	1.3635	1.2383	2.00	1.82	-9.18	78.10	Avg RF
Chrysene-d12	-----ISTD-----						
Pyrene	1.9954	1.8320	2.00	1.84	-8.19	77.86	Avg RF
Terphenyl-d14	0.7402	0.7260	2.00	1.96	-1.91	82.46	Avg RF
Benzo(a)Anthracene	0.9978	1.0912	2.00	1.79	10.50	71.35	Quadratic
Chrysene	0.9966	1.6085	2.00	1.96	2.17	77.50	Quadratic
Perylene-d12	-----ISTD-----						
Benzo(b)fluoranthene	1.7246	1.3886	2.00	1.61	-19.49	67.27	Avg RF
Benzo(k)fluoranthene	0.9999	1.6199	2.00	1.85	7.71	72.36	Quadratic
Benzo(a)pyrene	0.9996	1.1224	2.00	1.87	6.75	74.86	Quadratic
Indeno(1,2,3-cd)pyrene	1.1977	1.0048	2.00	1.68	-16.11	73.64	Avg RF
Dibenzo(a,h)anthracene	1.3915	1.2335	2.00	1.77	-11.36	76.99	Avg RF
Benzo(g,h,i)perylene	0.9993	1.4791	2.00	1.74	13.05	68.74	Quadratic

A -- against Average; M -- against Mid Point; P -- against Previous CC in the Method;

Audit Trail report

Batch name and path: \\MASSHUNTER\Org\Data\SV5975.I\sh011022\1 e8270d bna SIM\QuantResults\011022 bna SIM 1.batch.bin
Quant batch version: 10.0
Quant reporting version: 10.0

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdNewBatchTable	BL2000\jheine	1/10/2022 11:35:32 AM	Create new batch \\MASSHUNTER\Org\Data\SV5975.I\sh011022\1 e8270d bna SIM\011022 bna SIM 1.batch.bin			✓	
CmdImportSamplesFromWorklist	BL2000\jheine	1/10/2022 11:35:36 AM	Add samples from worklist: \\MASSHUNTER\Org\Data\SV5975.I\sh011022\1 e8270d bna SIM\Jan1001.D			✓	
CmdSetSampleAttribute	BL2000\jheine	1/10/2022 11:35:39 AM	Set SampleType = TuneCheck for sample Jan1001.D; previous value = Sample			✓	
CmdImportSamplesFromWorklist	BL2000\jheine	1/10/2022 12:06:39 PM	Add samples from worklist: \\MASSHUNTER\Org\Data\SV5975.I\sh011022\1 e8270d bna SIM\Jan1002.D			✓	
CmdStartMethodEditing	BL2000\jheine	1/10/2022 12:07:00 PM	Start method editing			✓	
CmdImportMethodFromBatch	BL2000\jheine	1/10/2022 12:07:01 PM	Import method from batch \\MASSHUNTER\Org\Data\SV5975.I\sh010522\3 e8270d bna SIM\010522 bna SIM 3.batch.bin			✓	
CmdApplyMethodToAllSamples	BL2000\jheine	1/10/2022 12:07:04 PM	Apply method to all samples			✓	
CmdMethodClear	BL2000\jheine	1/10/2022 12:07:05 PM	Clear method			✓	
CmdEndMethodEditing	BL2000\jheine	1/10/2022 12:07:05 PM	End method editing			✓	
CmdSetSampleAttribute	BL2000\jheine	1/10/2022 12:07:12 PM	Set SampleType = CC for sample Jan1002.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/10/2022 12:07:14 PM	Set LevelName = CCV for sample Jan1002.D; previous value =			✓	
CmdQuantitate	BL2000\jheine	1/10/2022 12:07:16 PM	Quantitate all compounds in sample Jan1002.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/10/2022 12:07:34 PM	Manually integrate compound Nitrobenzene-d5 in sample Jan1002.D, from x, y = 5.131, 501 to 5.417, 389, result = 5460; previous integration is from x, y = 5.131, 199 to 5.243, 211 and previous response = 8890.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/10/2022 12:07:36 PM	Snap baseline for compound Nitrobenzene-d5 in sample Jan1002.D, from x = 5.131 to x = 5.417, new integration is from x, y = 5.131, 181 to 5.417, 214 and new response = 9709; previous integration is from x, y = 5.131, 501 to 5.417, 389 and previous response = 5460.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/10/2022 12:07:41 PM	Set UserAnnotation = LT for compound Nitrobenzene-d5 in sample Jan1002.D; previous value =			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/10/2022 12:07:44 PM	Drop baseline for compound Nitrobenzene-d5 in sample Jan1002.D to y = 181, new integration is from x, y = 5.131, 181 to 5.417, 181 and new response = 9992; previous integration is from x, y = 5.131, 181 to 5.417, 214 and previous response = 9709.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/10/2022 12:07:55 PM	Manually integrate compound Benzo(b)fluoranthene in sample Jan1002.D, from x, y = 17.684, 59 to 17.783, 94, result = 19554; previous integration is from x, y = 17.711, 93 to 17.783, 100 and previous response = 19451.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/10/2022 12:07:58 PM	Drop baseline for compound Benzo(b)fluoranthene in sample Jan1002.D to y = 59, new integration is from x, y = 17.684, 59 to 17.783, 59 and new response = 19658; previous integration is from x, y = 17.684, 59 to 17.783, 94 and previous response = 19554.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/10/2022 12:07:59 PM	Set UserAnnotation = BA for compound Benzo(b)fluoranthene in sample Jan1002.D; previous value =			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/10/2022 12:08:20 PM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1002.D, from x, y = 5.953, 662 to 6.053, 93, result = 3298; previous integration is from x, y = 5.898, 93 to 6.053, 93 and previous response = 8611.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/10/2022 12:08:22 PM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1002.D to y = 93, new integration is from x, y = 5.953, 93 to 6.053, 93 and new response = 5005; previous integration is from x, y = 5.953, 662 to 6.053, 93 and previous response = 3298.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/10/2022 12:08:30 PM	Manually integrate qualifier 142.0 of compound 2-Methylnaphthalene in sample Jan1002.D from x, y = 6.777, 78 to 6.877, 4042; result = 9647			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/10/2022 12:08:32 PM	Drop baseline for qualifier 142.0 of compound 2-Methylnaphthalene in sample Jan1002.D to y = 78, new integration is from x, y = 6.777, 78 to 6.877, 78 and new response = 21528; previous integration is from x, y = 6.777, 78 to 6.877, 4042 and previous response = 9647.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/10/2022 12:08:41 PM	Manually integrate qualifier 142.0 of compound 1-Methylnaphthalene in sample Jan1002.D, from x, y = 6.890, 419 to 7.065, 78, result = 17929; previous integration is from x, y = 6.777, 78 to 7.065, 78 and previous response = 41796.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/10/2022 12:08:42 PM	Drop baseline for qualifier 142.0 of compound 1-Methylnaphthalene in sample Jan1002.D to y = 78, new integration is from x, y = 6.890, 78 to 7.065, 78 and new response = 19719; previous integration is from x, y = 6.890, 419 to 7.065, 78 and previous response = 17929.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/10/2022 12:08:52 PM	Manually integrate qualifier 153.0 of compound Acenaphthylene in sample Jan1002.D, from x, y = 7.813, 531 to 7.876, 2958, result = -2551; previous integration is from x, y = 8.025, 84 to 8.138, 84 and previous response = 20698.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/10/2022 12:08:54 PM	Snap baseline for qualifier 153.0 of compound Acenaphthylene in sample Jan1002.D from x = 7.813 to x = 7.876, new integration is from x, y = 7.813, 85 to 7.876, 240 and new response = 3365; previous integration is from x, y = 7.813, 531 to 7.876, 2958 and previous response = -2551.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/10/2022 12:08:55 PM	Snap baseline for qualifier 153.0 of compound Acenaphthylene in sample Jan1002.D from x = 7.813 to x = 7.876, new integration is from x, y = 7.813, 85 to 7.876, 240 and new response = 3365; previous integration is from x, y = 7.813, 85 to 7.876, 240 and previous response = 3365.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/10/2022 12:08:55 PM	Drop baseline for qualifier 153.0 of compound Acenaphthylene in sample Jan1002.D to y = 85, new integration is from x, y = 7.813, 85 to 7.876, 85 and new response = 3654; previous integration is from x, y = 7.813, 85 to 7.876, 240 and previous response = 3365.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/10/2022 12:09:38 PM	Manually integrate qualifier 152.0 of compound Acenaphthene in sample Jan1002.D, from x, y = 8.025, 3197 to 8.100, 5651, result = -9701; previous integration is from x, y = 7.813, 98 to 7.926, 98 and previous response = 27257.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/10/2022 12:09:39 PM	Snap baseline for qualifier 152.0 of compound Acenaphthene in sample Jan1002.D from x = 8.025 to x = 8.100, new integration is from x, y = 8.025, 135 to 8.100, 251 and new response = 9279; previous integration is from x, y = 8.025, 3197 to 8.100, 5651 and previous response = -9701.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/10/2022 12:09:40 PM	Drop baseline for qualifier 152.0 of compound Acenaphthene in sample Jan1002.D to y = 135, new integration is from x, y = 8.025, 135 to 8.100, 135 and new response = 9539; previous integration is from x, y = 8.025, 135 to 8.100, 251 and previous response = 9279.			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	1/10/2022 12:09:50 PM	Split qualifier 176.0 of compound Phenanthrene in sample Jan1002.D and keep left peak, new integration is from x, y = 9.780, 64.6809587374233 to 9.854, 64.6809587374233 and new response = 6120, previous integration is from x, y = 9.780, 65 to 9.904, 65 and previous response = 10815.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/10/2022 12:09:58 PM	Manually integrate qualifier 176.0 of compound Anthracene in sample Jan1002.D from x, y = 9.854, 564 to 9.953, 626; result = 2007			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/10/2022 12:09:59 PM	Snap baseline for qualifier 176.0 of compound Anthracene in sample Jan1002.D from x = 9.854 to x = 9.953, new integration is from x, y = 9.854, 186 to 9.953, 151 and new response = 4536; previous integration is from x, y = 9.854, 564 to 9.953, 626 and previous response = 2007.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/10/2022 12:10:00 PM	Drop baseline for qualifier 176.0 of compound Anthracene in sample Jan1002.D to y = 151, new integration is from x, y = 9.854, 151 to 9.953, 151 and new response = 4640; previous integration is from x, y = 9.854, 186 to 9.953, 151 and previous response = 4536.			✓	
CmdSaveBatchTable	BL2000\jheine	1/10/2022 12:10:33 PM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh011022\1 e8270d bna SIM\QuantResults\011022 bna SIM 1.batch.bin			✓	
CmdOpenBatchTable	BL2000\jheine	1/11/2022 8:22:01 AM	Open batch \\MASSHUNTER\Org\Data\SV5975.I\sh011022\1 e8270d bna SIM\011022 bna SIM 1.batch.bin			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdImportSamplesFromWorklist	BL2000\jheine	1/11/2022 8:23:09 AM	Add samples from worklist: \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\1 e8270d bna SIM\Jan1023.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\1 e8270d bna SIM\Jan1022.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\1 e8270d bna SIM\Jan1021.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\1 e8270d bna SIM\Jan1020.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\1 e8270d bna SIM\Jan1019.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\1 e8270d bna SIM\Jan1018.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\1 e8270d bna SIM\Jan1017.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\1 e8270d bna SIM\Jan1016.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\1 e8270d bna SIM\Jan1015.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\1 e8270d bna SIM\Jan1014.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\1 e8270d bna SIM\Jan1013.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\1 e8270d bna SIM\Jan1012.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\1 e8270d bna SIM\Jan1011.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\1 e8270d bna SIM\Jan1010.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\1 e8270d bna SIM\Jan1009.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\1 e8270d bna SIM\Jan1008.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\1 e8270d bna SIM\Jan1007.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\1 e8270d bna SIM\Jan1006.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\1 e8270d bna SIM\Jan1005.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\1 e8270d bna SIM\Jan1004.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\1 e8270d bna SIM\Jan1003.D			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:24:08 AM	Set SampleType = Blank for sample Jan1004.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:24:10 AM	Set SampleType = Calibration for sample Jan1005.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:24:13 AM	Set SampleType = Matrix for sample Jan1006.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:24:16 AM	Set SampleType = Blank for sample Jan1005.D; previous value = Calibration			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:24:21 AM	Set SampleType = MatrixDup for sample Jan1007.D; previous value = Sample			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:24:26 AM	Set SampleType = Matrix for sample Jan1016.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:24:29 AM	Set SampleType = Blank for sample Jan1017.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:24:31 AM	Set SampleType = Blank for sample Jan1018.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:24:39 AM	Set SampleType = Matrix for sample Jan1019.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:24:42 AM	Set SampleType = MatrixDup for sample Jan1020.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:24:46 AM	Set SampleType = CC for sample Jan1023.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:24:51 AM	Set LevelName = CCV for sample Jan1023.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:24:57 AM	Set MatrixSpikeGroup = MB-162701 for sample Jan1017.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:24:59 AM	Set MatrixSpikeGroup = MB-162701 for sample Jan1019.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:25:00 AM	Set MatrixSpikeGroup = MB-162701 for sample Jan1020.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:25:08 AM	Set MatrixSpikeGroup = B21122105-001C for sample Jan1014.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:25:09 AM	Set MatrixSpikeGroup = B21122105-001C for sample Jan1016.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:25:14 AM	Set MatrixSpikeGroup = MB-162577 for sample Jan1004.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:25:16 AM	Set MatrixSpikeGroup = MB-162577 for sample Jan1006.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:25:17 AM	Set MatrixSpikeGroup = MB-162577 for sample Jan1007.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:25:22 AM	Set SampleInformation = MatrixA for sample Jan1006.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:25:26 AM	Set SampleInformation = MatrixA for sample Jan1007.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:25:29 AM	Set SampleInformation = MatrixA for sample Jan1019.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:25:31 AM	Set SampleInformation = MatrixA for sample Jan1020.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:25:32 AM	Set SampleInformation = MatrixA for sample Jan1016.D; previous value =			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdQuantitate	BL2000\jheine	1/11/2022 8:25:41 AM	Quantitate all compounds in all samples			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:26:01 AM	Manually integrate compound Benzo(a)pyrene in sample Jan1003.D, from x, y = 18.376, 85 to 18.450, 220, result = -350; previous integration is from x, y = 18.476, 61 to 18.660, 73 and previous response = 1653.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/11/2022 8:26:03 AM	Snap baseline for compound Benzo(a)pyrene in sample Jan1003.D, from x = 18.376 to x = 18.450, new integration is from x, y = 18.376, 59 to 18.450, 59 and new response = 66; previous integration is from x, y = 18.376, 85 to 18.450, 220 and previous response = -350.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:26:04 AM	Drop baseline for compound Benzo(a)pyrene in sample Jan1003.D to y = 59, new integration is from x, y = 18.376, 59 to 18.450, 59 and new response = 66; previous integration is from x, y = 18.376, 59 to 18.450, 59 and previous response = 66.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:26:06 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1003.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:26:11 AM	Manually integrate compound Acenaphthene in sample Jan1003.D, from x, y = 8.038, 368 to 8.075, 71, result = -191; previous integration is from x, y = 7.989, 71 to 8.075, 71 and previous response = 1478.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:26:12 AM	Drop baseline for compound Acenaphthene in sample Jan1003.D to y = 71, new integration is from x, y = 8.038, 71 to 8.075, 71 and new response = 143; previous integration is from x, y = 8.038, 368 to 8.075, 71 and previous response = -191.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:26:14 AM	Zero out primary peak of compound Acenaphthene in sample Jan1003.D			✓	
CmdClearManualIntegration	BL2000\jheine	1/11/2022 8:26:23 AM	Clear manual integration of target signal for compound Acenaphthene in sample Jan1003.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:26:28 AM	Manually integrate compound Acenaphthene in sample Jan1003.D, from x, y = 8.038, 326 to 8.075, 71, result = -144; previous integration is from x, y = 7.989, 71 to 8.075, 71 and previous response = 1478.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:26:29 AM	Drop baseline for compound Acenaphthene in sample Jan1003.D to y = 71, new integration is from x, y = 8.038, 71 to 8.075, 71 and new response = 143; previous integration is from x, y = 8.038, 326 to 8.075, 71 and previous response = -144.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:26:32 AM	Zero out primary peak of compound Acenaphthene in sample Jan1003.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:26:37 AM	Manually integrate compound Chrysene in sample Jan1003.D, from x, y = 14.789, 101 to 14.888, 54, result = 202; previous integration is from x, y = 14.689, 54 to 14.888, 54 and previous response = 1993.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:26:39 AM	Drop baseline for compound Chrysene in sample Jan1003.D to y = 54, new integration is from x, y = 14.789, 54 to 14.888, 54 and new response = 341; previous integration is from x, y = 14.789, 101 to 14.888, 54 and previous response = 202.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:26:40 AM	Zero out primary peak of compound Chrysene in sample Jan1003.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:26:44 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1003.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:26:56 AM	Manually integrate compound Fluorene in sample Jan1004.D, from x, y = 8.661, 70 to 8.711, 90, result = 214; previous integration is from x, y = 8.960, 70 to 9.072, 70 and previous response = 11393.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:26:57 AM	Drop baseline for compound Fluorene in sample Jan1004.D to y = 70, new integration is from x, y = 8.661, 70 to 8.711, 70 and new response = 244; previous integration is from x, y = 8.661, 70 to 8.711, 90 and previous response = 214.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:26:59 AM	Zero out primary peak of compound Fluorene in sample Jan1004.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:27:07 AM	Manually integrate compound Benzo(a)pyrene in sample Jan1004.D, from x, y = 18.376, 65 to 18.450, 71, result = 175; previous integration is from x, y = 18.477, 72 to 18.647, 73 and previous response = 1693.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:27:09 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1004.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:27:15 AM	Manually integrate compound Acenaphthene in sample Jan1004.D, from x, y = 8.038, 126 to 8.075, 78, result = 205; previous integration is from x, y = 7.988, 78 to 8.075, 78 and previous response = 1670.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:27:16 AM	Drop baseline for compound Acenaphthene in sample Jan1004.D to y = 78, new integration is from x, y = 8.038, 78 to 8.075, 78 and new response = 260; previous integration is from x, y = 8.038, 126 to 8.075, 78 and previous response = 205.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:27:19 AM	Zero out primary peak of compound Acenaphthene in sample Jan1004.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:27:25 AM	Manually integrate compound Chrysene in sample Jan1004.D, from x, y = 14.789, 191 to 14.901, 197, result = -255; previous integration is from x, y = 14.684, 56 to 14.789, 57 and previous response = 2006.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/11/2022 8:27:27 AM	Snap baseline for compound Chrysene in sample Jan1004.D, from x = 14.789 to x = 14.901, new integration is from x, y = 14.789, 166 to 14.901, 82 and new response = 217; previous integration is from x, y = 14.789, 191 to 14.901, 197 and previous response = -255.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:27:28 AM	Drop baseline for compound Chrysene in sample Jan1004.D to y = 82, new integration is from x, y = 14.789, 82 to 14.901, 82 and new response = 500; previous integration is from x, y = 14.789, 166 to 14.901, 82 and previous response = 217.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:27:29 AM	Zero out primary peak of compound Chrysene in sample Jan1004.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:27:32 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1004.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:27:53 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1005.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:27:58 AM	Manually integrate compound Acenaphthene in sample Jan1005.D, from x, y = 8.038, 357 to 8.100, 69, result = -343; previous integration is from x, y = 7.988, 69 to 8.100, 69 and previous response = 1597.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:28:00 AM	Drop baseline for compound Acenaphthene in sample Jan1005.D to y = 69, new integration is from x, y = 8.038, 69 to 8.100, 69 and new response = 196; previous integration is from x, y = 8.038, 357 to 8.100, 69 and previous response = -343.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:28:01 AM	Zero out primary peak of compound Acenaphthene in sample Jan1005.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:28:05 AM	Zero out primary peak of compound Chrysene in sample Jan1005.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:28:06 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1005.D			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/11/2022 8:28:23 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1006.D, from x, y = 5.953, 785 to 6.041, 83, result = 4593; previous integration is from x, y = 5.903, 83 to 6.041, 83 and previous response = 11038.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:28:24 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1006.D to y = 83, new integration is from x, y = 5.953, 83 to 6.041, 83 and new response = 6434; previous integration is from x, y = 5.953, 785 to 6.041, 83 and previous response = 4593.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/11/2022 8:29:16 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1007.D, from x, y = 5.953, 659 to 6.041, 87, result = 3827; previous integration is from x, y = 5.880, 87 to 6.041, 87 and previous response = 9811.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:29:17 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1007.D to y = 87, new integration is from x, y = 5.953, 87 to 6.041, 87 and new response = 5325; previous integration is from x, y = 5.953, 659 to 6.041, 87 and previous response = 3827.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:29:57 AM	Manually integrate compound Benzo(g,h,i)perylene in sample Jan1007.D, from x, y = 20.550, 4957 to 20.699, 7406, result = 12347; previous integration is from x, y = 20.553, 2042 to 20.641, 1886 and previous response = 51010.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/11/2022 8:29:58 AM	Snap baseline for compound Benzo(g,h,i)perylene in sample Jan1007.D, from x = 20.550 to x = 20.699, new integration is from x, y = 20.550, 347 to 20.699, 728 and new response = 62562; previous integration is from x, y = 20.550, 4957 to 20.699, 7406 and previous response = 12347.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:29:59 AM	Drop baseline for compound Benzo(g,h,i)perylene in sample Jan1007.D to y = 347, new integration is from x, y = 20.550, 347 to 20.699, 347 and new response = 64257; previous integration is from x, y = 20.550, 347 to 20.699, 728 and previous response = 62562.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/11/2022 8:30:00 AM	Set UserAnnotation = BA for compound Benzo(g,h,i)perylene in sample Jan1007.D; previous value =			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:30:13 AM	Zero out primary peak of compound Fluorene in sample Jan1008.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:30:16 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1008.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:30:22 AM	Manually integrate compound Acenaphthene in sample Jan1008.D, from x, y = 8.038, 87 to 8.088, 73, result = 120; previous integration is from x, y = 7.976, 73 to 8.088, 73 and previous response = 1568.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:30:23 AM	Drop baseline for compound Acenaphthene in sample Jan1008.D to y = 73, new integration is from x, y = 8.038, 73 to 8.088, 73 and new response = 142; previous integration is from x, y = 8.038, 87 to 8.088, 73 and previous response = 120.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:30:25 AM	Zero out primary peak of compound Acenaphthene in sample Jan1008.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:30:28 AM	Zero out primary peak of compound Chrysene in sample Jan1008.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:30:30 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1008.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:30:49 AM	Manually integrate compound Benzo(a)pyrene in sample Jan1009.D, from x, y = 18.388, 93 to 18.438, 182, result = -172; previous integration is from x, y = 18.476, 66 to 18.672, 68 and previous response = 1636.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/11/2022 8:30:50 AM	Snap baseline for compound Benzo(a)pyrene in sample Jan1009.D, from x = 18.388 to x = 18.438, new integration is from x, y = 18.388, 64 to 18.438, 65 and new response = 46; previous integration is from x, y = 18.388, 93 to 18.438, 182 and previous response = -172.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:30:51 AM	Drop baseline for compound Benzo(a)pyrene in sample Jan1009.D to y = 64, new integration is from x, y = 18.388, 64 to 18.438, 64 and new response = 47; previous integration is from x, y = 18.388, 64 to 18.438, 65 and previous response = 46.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:30:53 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1009.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:30:59 AM	Manually integrate compound Acenaphthene in sample Jan1009.D, from x, y = 8.038, 88 to 8.100, 66, result = 122; previous integration is from x, y = 7.989, 66 to 8.100, 66 and previous response = 1437.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:31:00 AM	Drop baseline for compound Acenaphthene in sample Jan1009.D to y = 66, new integration is from x, y = 8.038, 66 to 8.100, 66 and new response = 162; previous integration is from x, y = 8.038, 88 to 8.100, 66 and previous response = 122.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:31:01 AM	Zero out primary peak of compound Acenaphthene in sample Jan1009.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:31:07 AM	Manually integrate compound Chrysene in sample Jan1009.D, from x, y = 14.789, 105 to 14.876, 54, result = 165; previous integration is from x, y = 14.688, 53 to 14.876, 54 and previous response = 2005.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:31:09 AM	Drop baseline for compound Chrysene in sample Jan1009.D to y = 54, new integration is from x, y = 14.789, 54 to 14.876, 54 and new response = 299; previous integration is from x, y = 14.789, 105 to 14.876, 54 and previous response = 165.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:31:11 AM	Zero out primary peak of compound Chrysene in sample Jan1009.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:31:13 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1009.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:31:33 AM	Manually integrate compound Fluorene in sample Jan1010.D, from x, y = 8.661, 73 to 8.723, 74, result = 76; previous integration is from x, y = 8.955, 73 to 9.072, 77 and previous response = 12281.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:31:34 AM	Zero out primary peak of compound Fluorene in sample Jan1010.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:31:40 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1010.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:31:45 AM	Manually integrate compound Acenaphthene in sample Jan1010.D, from x, y = 8.038, 114 to 8.100, 79, result = 62; previous integration is from x, y = 7.984, 79 to 8.100, 79 and previous response = 1553.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:31:47 AM	Drop baseline for compound Acenaphthene in sample Jan1010.D to y = 79, new integration is from x, y = 8.038, 79 to 8.100, 79 and new response = 127; previous integration is from x, y = 8.038, 114 to 8.100, 79 and previous response = 62.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:31:48 AM	Zero out primary peak of compound Acenaphthene in sample Jan1010.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:31:52 AM	Zero out primary peak of compound Chrysene in sample Jan1010.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:31:54 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1010.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:32:11 AM	Manually integrate compound Benzo(a)pyrene in sample Jan1011.D, from x, y = 18.388, 101 to 18.450, 184, result = -242; previous integration is from x, y = 18.475, 62 to 18.610, 63 and previous response = 1888.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/11/2022 8:32:12 AM	Snap baseline for compound Benzo(a)pyrene in sample Jan1011.D, from x = 18.388 to x = 18.450, new integration is from x, y = 18.388, 59 to 18.450, 64 and new response = 59; previous integration is from x, y = 18.388, 101 to 18.450, 184 and previous response = -242.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:32:13 AM	Drop baseline for compound Benzo(a)pyrene in sample Jan1011.D to y = 59, new integration is from x, y = 18.388, 59 to 18.450, 59 and new response = 68; previous integration is from x, y = 18.388, 59 to 18.450, 64 and previous response = 59.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:32:15 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1011.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:32:21 AM	Manually integrate compound Acenaphthene in sample Jan1011.D, from x, y = 8.038, 308 to 8.100, 67, result = -279; previous integration is from x, y = 7.989, 67 to 8.100, 67 and previous response = 1596.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:32:22 AM	Drop baseline for compound Acenaphthene in sample Jan1011.D to y = 67, new integration is from x, y = 8.038, 67 to 8.100, 67 and new response = 171; previous integration is from x, y = 8.038, 308 to 8.100, 67 and previous response = -279.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:32:23 AM	Zero out primary peak of compound Acenaphthene in sample Jan1011.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:32:26 AM	Zero out primary peak of compound Chrysene in sample Jan1011.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:32:27 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1011.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:32:38 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1012.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:32:40 AM	Zero out primary peak of compound Acenaphthene in sample Jan1012.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:32:41 AM	Zero out primary peak of compound Chrysene in sample Jan1012.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:32:43 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1012.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:32:59 AM	Manually integrate compound Benzo(a)pyrene in sample Jan1013.D, from x, y = 18.388, 80 to 18.437, 150, result = -111; previous integration is from x, y = 18.479, 64 to 18.586, 66 and previous response = 1736.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/11/2022 8:33:00 AM	Snap baseline for compound Benzo(a)pyrene in sample Jan1013.D, from x = 18.388 to x = 18.437, new integration is from x, y = 18.388, 60 to 18.437, 64 and new response = 47; previous integration is from x, y = 18.388, 80 to 18.437, 150 and previous response = -111.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:33:01 AM	Drop baseline for compound Benzo(a)pyrene in sample Jan1013.D to y = 60, new integration is from x, y = 18.388, 60 to 18.437, 60 and new response = 53; previous integration is from x, y = 18.388, 60 to 18.437, 64 and previous response = 47.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:33:02 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1013.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:33:08 AM	Manually integrate compound Acenaphthene in sample Jan1013.D, from x, y = 8.038, 87 to 8.088, 65, result = 135; previous integration is from x, y = 7.988, 65 to 8.088, 65 and previous response = 1490.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:33:09 AM	Drop baseline for compound Acenaphthene in sample Jan1013.D to y = 65, new integration is from x, y = 8.038, 65 to 8.088, 65 and new response = 168; previous integration is from x, y = 8.038, 87 to 8.088, 65 and previous response = 135.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:33:11 AM	Zero out primary peak of compound Acenaphthene in sample Jan1013.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:33:13 AM	Zero out primary peak of compound Chrysene in sample Jan1013.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:33:14 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1013.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:33:30 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1014.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:33:32 AM	Zero out primary peak of compound Acenaphthene in sample Jan1014.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:33:34 AM	Zero out primary peak of compound Chrysene in sample Jan1014.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:33:35 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1014.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:36:24 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1015.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:36:29 AM	Manually integrate compound Acenaphthene in sample Jan1015.D, from x, y = 8.038, 316 to 8.075, 66, result = -141; previous integration is from x, y = 7.988, 66 to 8.075, 66 and previous response = 1589.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:36:30 AM	Drop baseline for compound Acenaphthene in sample Jan1015.D to y = 66, new integration is from x, y = 8.038, 66 to 8.075, 66 and new response = 138; previous integration is from x, y = 8.038, 316 to 8.075, 66 and previous response = -141.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:36:31 AM	Zero out primary peak of compound Acenaphthene in sample Jan1015.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:36:33 AM	Zero out primary peak of compound Chrysene in sample Jan1015.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/11/2022 8:36:51 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1016.D, from x, y = 5.953, 750 to 6.053, 88, result = 4848; previous integration is from x, y = 5.884, 88 to 6.053, 88 and previous response = 10965.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:36:52 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1016.D to y = 88, new integration is from x, y = 5.953, 88 to 6.053, 88 and new response = 6831; previous integration is from x, y = 5.953, 750 to 6.053, 88 and previous response = 4848.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:37:42 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1017.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:37:47 AM	Manually integrate compound Acenaphthene in sample Jan1017.D, from x, y = 8.038, 145 to 8.088, 78, result = 34; previous integration is from x, y = 7.988, 79 to 8.088, 78 and previous response = 1507.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:37:49 AM	Drop baseline for compound Acenaphthene in sample Jan1017.D to y = 78, new integration is from x, y = 8.038, 78 to 8.088, 78 and new response = 134; previous integration is from x, y = 8.038, 145 to 8.088, 78 and previous response = 34.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:37:50 AM	Zero out primary peak of compound Acenaphthene in sample Jan1017.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:37:53 AM	Zero out primary peak of compound Chrysene in sample Jan1017.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:37:55 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1017.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:38:10 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1018.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:38:16 AM	Manually integrate compound Acenaphthene in sample Jan1018.D, from x, y = 8.038, 106 to 8.100, 65, result = 98; previous integration is from x, y = 7.981, 65 to 8.100, 65 and previous response = 1590.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:38:18 AM	Drop baseline for compound Acenaphthene in sample Jan1018.D to y = 65, new integration is from x, y = 8.038, 65 to 8.100, 65 and new response = 174; previous integration is from x, y = 8.038, 106 to 8.100, 65 and previous response = 98.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:38:19 AM	Zero out primary peak of compound Acenaphthene in sample Jan1018.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:38:22 AM	Zero out primary peak of compound Chrysene in sample Jan1018.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:38:23 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1018.D			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/11/2022 8:38:36 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1019.D, from x, y = 5.953, 619 to 6.053, 103, result = 5710; previous integration is from x, y = 5.916, 106 to 6.053, 103 and previous response = 11325.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:38:38 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1019.D to y = 103, new integration is from x, y = 5.953, 103 to 6.053, 103 and new response = 7255; previous integration is from x, y = 5.953, 619 to 6.053, 103 and previous response = 5710.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/11/2022 8:39:31 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1020.D, from x, y = 5.953, 649 to 6.053, 87, result = 6592; previous integration is from x, y = 5.884, 87 to 6.053, 87 and previous response = 12884.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:39:33 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1020.D to y = 87, new integration is from x, y = 5.953, 87 to 6.053, 87 and new response = 8275; previous integration is from x, y = 5.953, 649 to 6.053, 87 and previous response = 6592.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:40:24 AM	Manually integrate compound Fluorene in sample Jan1021.D, from x, y = 8.673, 75 to 8.711, 189, result = -77; previous integration is from x, y = 8.960, 67 to 9.147, 71 and previous response = 12616.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/11/2022 8:40:25 AM	Snap baseline for compound Fluorene in sample Jan1021.D, from x = 8.673 to x = 8.711, new integration is from x, y = 8.673, 75 to 8.711, 75 and new response = 51; previous integration is from x, y = 8.673, 75 to 8.711, 189 and previous response = -77.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:40:26 AM	Drop baseline for compound Fluorene in sample Jan1021.D to y = 75, new integration is from x, y = 8.673, 75 to 8.711, 75 and new response = 51; previous integration is from x, y = 8.673, 75 to 8.711, 75 and previous response = 51.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:40:28 AM	Zero out primary peak of compound Fluorene in sample Jan1021.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:40:31 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1021.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:40:35 AM	Zero out primary peak of compound Acenaphthene in sample Jan1021.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:40:38 AM	Zero out primary peak of compound Chrysene in sample Jan1021.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:40:39 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1021.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:40:58 AM	Manually integrate compound Benzo(a)pyrene in sample Jan1022.D, from x, y = 18.388, 104 to 18.450, 198, result = -262; previous integration is from x, y = 18.475, 60 to 18.648, 76 and previous response = 1965.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/11/2022 8:41:00 AM	Snap baseline for compound Benzo(a)pyrene in sample Jan1022.D, from x = 18.388 to x = 18.450, new integration is from x, y = 18.388, 68 to 18.450, 62 and new response = 56; previous integration is from x, y = 18.388, 104 to 18.450, 198 and previous response = -262.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:41:00 AM	Drop baseline for compound Benzo(a)pyrene in sample Jan1022.D to y = 62, new integration is from x, y = 18.388, 62 to 18.450, 62 and new response = 67; previous integration is from x, y = 18.388, 68 to 18.450, 62 and previous response = 56.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:41:02 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1022.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:41:07 AM	Manually integrate compound Acenaphthene in sample Jan1022.D, from x, y = 8.038, 281 to 8.088, 68, result = -158; previous integration is from x, y = 7.989, 68 to 8.088, 68 and previous response = 1551.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:41:09 AM	Drop baseline for compound Acenaphthene in sample Jan1022.D to y = 68, new integration is from x, y = 8.038, 68 to 8.088, 68 and new response = 160; previous integration is from x, y = 8.038, 281 to 8.088, 68 and previous response = -158.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:41:10 AM	Zero out primary peak of compound Acenaphthene in sample Jan1022.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:41:13 AM	Zero out primary peak of compound Chrysene in sample Jan1022.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:41:15 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1022.D			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/11/2022 8:41:31 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1023.D, from x, y = 5.953, 2449 to 6.040, 2629, result = -8729; previous integration is from x, y = 5.905, 84 to 6.178, 84 and previous response = 8845.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/11/2022 8:41:32 AM	Snap baseline for qualifier 102.0 of compound Naphthalene in sample Jan1023.D from x = 5.953 to x = 6.040, new integration is from x, y = 5.953, 1322 to 6.040, 116 and new response = 815; previous integration is from x, y = 5.953, 2449 to 6.040, 2629 and previous response = -8729.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:41:33 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1023.D to y = 116, new integration is from x, y = 5.953, 116 to 6.040, 116 and new response = 3978; previous integration is from x, y = 5.953, 1322 to 6.040, 116 and previous response = 815.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/11/2022 8:41:50 AM	Manually integrate qualifier 152.0 of compound Acenaphthene in sample Jan1023.D from x, y = 8.025, 3389 to 8.113, 5106; result = -12689			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/11/2022 8:41:51 AM	Snap baseline for qualifier 152.0 of compound Acenaphthene in sample Jan1023.D from x = 8.025 to x = 8.113, new integration is from x, y = 8.025, 125 to 8.113, 181 and new response = 8743; previous integration is from x, y = 8.025, 3389 to 8.113, 5106 and previous response = -12689.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:41:52 AM	Drop baseline for qualifier 152.0 of compound Acenaphthene in sample Jan1023.D to y = 125, new integration is from x, y = 8.025, 125 to 8.113, 125 and new response = 8889; previous integration is from x, y = 8.025, 125 to 8.113, 181 and previous response = 8743.			✓	
CmdSaveBatchTable	BL2000\jheine	1/11/2022 8:42:26 AM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh011022\1 e8270d bna SIM\QuantResults\011022 bna SIM 1.batch.bin			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:43:05 AM	Set SampleApproved = True for sample Jan1001.D; previous value = False			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:43:06 AM	Set SampleApproved = True for sample Jan1002.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:43:08 AM	Set SampleApproved = True for sample Jan1003.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:43:09 AM	Set SampleApproved = True for sample Jan1004.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:43:10 AM	Set SampleApproved = True for sample Jan1005.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:43:12 AM	Set SampleApproved = True for sample Jan1006.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:43:13 AM	Set SampleApproved = True for sample Jan1007.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:43:14 AM	Set SampleApproved = True for sample Jan1008.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:43:15 AM	Set SampleApproved = True for sample Jan1009.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:43:17 AM	Set SampleApproved = True for sample Jan1010.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:43:17 AM	Set SampleApproved = True for sample Jan1011.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:43:18 AM	Set SampleApproved = True for sample Jan1012.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:43:20 AM	Set SampleApproved = True for sample Jan1013.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:43:21 AM	Set SampleApproved = True for sample Jan1014.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:43:22 AM	Set SampleApproved = True for sample Jan1015.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:43:23 AM	Set SampleApproved = True for sample Jan1016.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:43:24 AM	Set SampleApproved = True for sample Jan1017.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:43:27 AM	Set SampleApproved = True for sample Jan1018.D; previous value = False			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:43:29 AM	Set SampleApproved = True for sample Jan1019.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:43:31 AM	Set SampleApproved = True for sample Jan1020.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:43:32 AM	Set SampleApproved = True for sample Jan1021.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:43:33 AM	Set SampleApproved = True for sample Jan1022.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:43:34 AM	Set SampleApproved = True for sample Jan1023.D; previous value = False			✓	
CmdSaveBatchTable	BL2000\jheine	1/11/2022 8:43:37 AM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\1 e8270d bna SIM\QuantResults\011022 bna SIM 1.batch.bin			✓	
CmdSaveBatchTable	BL2000\jheine	1/11/2022 8:44:06 AM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\1 e8270d bna SIM\QuantResults\011022 bna SIM 1.batch.bin			✓	
CmdSaveBatchTable	BL2000\jheine	1/11/2022 8:45:02 AM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\1 e8270d bna SIM\QuantResults\011022 bna SIM 1.batch.bin			✓	
CmdOpenBatchTable	BL2000\jheine	1/19/2022 5:04:28 PM	Open batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\1 e8270d bna SIM\011022 bna SIM 1.batch.bin			✓	
CmdQuantitate	BL2000\jheine	1/19/2022 5:05:03 PM	Quantitate all compounds in all samples			✓	
CmdSaveBatchTable	BL2000\jheine	1/19/2022 5:05:13 PM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\1 e8270d bna SIM\QuantResults\011022 bna SIM 1.batch.bin			✓	
GenerateReport	BL2000\jheine	1/19/2022 5:14:27 PM	Generates report - Method: D:\Org\reports\GCMSEMI Report Templates\Tests_for_LevelIV\Env_Qua ntResults_wGraphics+Chromatogram. m, Output Path: \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\1 e8270d bna SIM\QuantReports\			✓	

Energy Laboratories Inc

ANALYTICAL RUN Summary

19-Jan-22

Run ID SV5975.I_220110B

Run Start Date: 1/10/2022
Analyst: John P. Heine
Ical:
Column ID: ZB-SemiVolatiles
Comments:

Std ID	Std Name	Std Amount	Std Units	Samp Amount	Samp Units	SampType	Expiration Date
dcmsvoc13	DCM						11/17/2022
sv100210	BNA 2nd source 200ug/mL	2	ul	198	ul	ICV	1/15/2022
sv100506	BNA low 50 ug/mL	8	ul	192	ul	CCV	3/31/2022
sv100703	BNA Internals 2000 ug/mL	2	ul	100	ul	SAMP	5/31/2022
sv83311	DFTPP 1000 ug/mL	50	ul	50	ul	TUNE	10/31/2022

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14972034	Jan1024_D_TU	SVOC-8270-DF	TUNE	√5975.I\sh0110221	10/2022 11:36:	1	R372988		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
127, % of mass 198	A	%	54.8	54.8		100	0	0	0	0.01	0	55%	40	60	0%	
197, % of mass 198	A	%	0	0		100	0	0	0	0.01	0	0%	0	0.99	0%	
198, Base Peak	A	%	100	100		100	0	0	0	0.01	0	100%	100	100	0%	
199, % of mass 198	A	%	6.7	6.7		100	0	0	0	0.01	0	7%	5	9	0%	
275, % of mass 198	A	%	28.9	28.9		100	0	0	0	0.01	0	29%	10	30	0%	
365, % of mass 198	A	%	3.2	3.2		100	0	0	0	0.01	0	3%	1	99.99	0%	
441, % of mass 443	A	%	93.6	93.6		100	0	0	0	0.01	0	94%	0.01	150	0%	
442, % of mass 198	A	%	64.7	64.7		100	0	0	0	0.01	0	65%	40	100	0%	
443, % of mass 442	A	%	18.8	18.8		100	0	0	0	0.01	0	19%	17	23	0%	
51, % of mass 198	A	%	51.3	51.3		100	0	0	0	0.01	0	51%	30	60	0%	
68, % of mass 69	A	%	0	0		100	0	0	0	0.01	0	0%	0	1.99	0%	
70, % of mass 69	A	%	0.4	0.4		100	0	0	0	0.01	0	0%	0	1.99	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14973248	10-Jan-22_CC	SVOC-8270-W-	CCV	v5975.I\sh0110221/10/2022	11:59:	1	R372988		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	2.35717	2.35717		2	0	0	0.0206	0.1	10	118%	80	120	0%	
2-Methylnaphthalene	A	ug/L	2.09598	2.09598		2	0	0	0.0176	0.1	10	105%	80	120	0%	
Acenaphthene	A	ug/L	1.71855	1.71855		2	0	0	0.0317	0.1	10	86%	80	120	0%	
Acenaphthylene	A	ug/L	1.92929	1.92929		2	0	0	0.025	0.1	10	96%	80	120	0%	
Anthracene	A	ug/L	2.05066	2.05066		2	0	0	0.0283	0.1	10	103%	80	120	0%	
Benzo(a)anthracene	A	ug/L	1.91912	1.91912		2	0	0	0.0272	0.1	10	96%	80	120	0%	
Benzo(a)pyrene	A	ug/L	1.88032	1.88032		2	0	0	0.0347	0.1	10	94%	80	120	0%	
Benzo(b)fluoranthene	A	ug/L	1.70536	1.70536		2	0	0	0.0226	0.1	10	85%	80	120	0%	
Benzo(g,h,i)perylene	A	ug/L	1.94311	1.94311		2	0	0	0.0267	0.1	10	97%	80	120	0%	
Benzo(k)fluoranthene	A	ug/L	1.99827	1.99827		2	0	0	0.0295	0.1	10	100%	80	120	0%	
Chrysene	A	ug/L	1.9925	1.9925		2	0	0	0.0458	0.1	10	100%	80	120	0%	
Dibenzo(a,h)anthracene	A	ug/L	1.79461	1.79461		2	0	0	0.0367	0.1	10	90%	80	120	0%	
Fluoranthene	A	ug/L	1.9127	1.9127		2	0	0	0.0233	0.1	10	96%	80	120	0%	
Fluorene	A	ug/L	2.01922	2.01922		2	0	0	0.0225	0.1	10	101%	80	120	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	1.68367	1.68367		2	0	0	0.0491	0.1	10	84%	80	120	0%	
Naphthalene	A	ug/L	1.93409	1.93409		2	0	0	0.029	0.1	10	97%	80	120	0%	
Phenanthrene	A	ug/L	2.00983	2.00983		2	0	0	0.0295	0.1	10	100%	80	120	0%	
Pyrene	A	ug/L	1.84756	1.84756		2	0	0	0.0239	0.1	10	92%	80	120	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
2-Fluorobiphenyl	S	ug/L	1.94547	1.94547		2	0	0	0.0444	0.1	10	97%	80	120	0%	
Nitrobenzene-d5	S	ug/L	1.7365	1.7365		2	0	0	0.0523	0.1	10	87%	80	120	0%	
Terphenyl-d14	S	ug/L	2.02994	2.02994		2	0	0	0.0563	0.1	10	101%	80	120	0%	
o-Terphenyl	X	ug/L	1.82838	1.82838		2	0	0	0.0654	0.1	10	91%	80	120	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14973249	10-Jan-22_ISTB	SVOC-8270-W-	SAMP	v5975.I\sh0110221/11/2022	12:31:	1	R372988		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14973249	10-Jan-22_ISTB	SVOC-8270-W-	SAMP	v5975.I\sh0110221/11/2022	12:31:	1	R372988		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0206	0.1	10	0%	0	0	0%	
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0176	0.1	10	0%	0	0	0%	
Acenaphthene	A	ug/L	0	0		0	0	0	0.0317	0.1	10	0%	0	0	0%	
Acenaphthylene	A	ug/L	0	0		0	0	0	0.025	0.1	10	0%	0	0	0%	
Anthracene	A	ug/L	0	0		0	0	0	0.0283	0.1	10	0%	0	0	0%	
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.0272	0.1	10	0%	0	0	0%	
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.0347	0.1	10	0%	0	0	0%	
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.0226	0.1	10	0%	0	0	0%	
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.0267	0.1	10	0%	0	0	0%	
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.0295	0.1	10	0%	0	0	0%	
Chrysene	A	ug/L	0	0		0	0	0	0.0458	0.1	10	0%	0	0	0%	
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.0367	0.1	10	0%	0	0	0%	
Fluoranthene	A	ug/L	0	0		0	0	0	0.0233	0.1	10	0%	0	0	0%	
Fluorene	A	ug/L	0	0		0	0	0	0.0225	0.1	10	0%	0	0	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.0491	0.1	10	0%	0	0	0%	
Naphthalene	A	ug/L	0	0		0	0	0	0.029	0.1	10	0%	0	0	0%	
Phenanthrene	A	ug/L	0	0		0	0	0	0.0295	0.1	10	0%	0	0	0%	
Pyrene	A	ug/L	0	0		0	0	0	0.0239	0.1	10	0%	0	0	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
2-Fluorobiphenyl	S	ug/L	0	0		5	0	0	0.0444	0.1	10	0%	25	94	0%	S
Nitrobenzene-d5	S	ug/L	0	0		5	0	0	0.0523	0.1	10	0%	19	102	0%	S
Terphenyl-d14	S	ug/L	0	0		5	0	0	0.0563	0.1	10	0%	39	106	0%	S
o-Terphenyl	X	ug/L	0	0		200	0	0	0.0654	0.1	10	0%	40	140	0%	S

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14973250	B22010120-001	SVOC-8270-W-	SAMP	v5975.I\sh0110221/11/2022	1:04:1	1	162701	1/4/2022 3:4	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14973250	B22010120-001	SVOC-8270-W-	SAMP	√5975.I\sh0110221/11/2022	1:04:1	1	162701	1/4/2022 3:4	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0200026	0.1	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0170896	0.1	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.0307807	0.1	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.024275	0.1	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.0274793	0.1	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.0264112	0.1	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.0336937	0.1	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.0219446	0.1	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.0259257	0.1	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.0286445	0.1	10	0%	0	0	0%	U
Chrysene	A	ug/L	0	0		0	0	0	0.0444718	0.1	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.0356357	0.1	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0	0		0	0	0	0.0226243	0.1	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.0218475	0.1	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.0476761	0.1	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.028159	0.1	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.0286445	0.1	10	0%	0	0	0%	U
Pyrene	A	ug/L	0	0		0	0	0	0.0232069	0.1	10	0%	0	0	0%	U
1,4-Dichlorobenzene-d4	I	ug/L	40	38.84		0	0	0	0.0971	0.1		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	38.84		0	0	0	0.0971	0.1		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	38.84		0	0	0	0.0971	0.1		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	38.84		0	0	0	0.0971	0.1		0%	0	0	0%	
Perylene-d12	I	ug/L	40	38.84		0	0	0	0.0971	0.1		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	38.84		0	0	0	0.0971	0.1		0%	0	0	0%	
o-Terphenyl	X	ug/L	0	0		194.2	0	0	0.0635034	0.1	10	0%	40	140	0%	US

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14973251	B22010120-001	SVOC-8270-W-	SAMP	√5975.I\sh0110221/11/2022	1:36:4	20	162701	1/4/2022 3:4	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
2-Fluorobiphenyl	S	ug/L	3.92547	76.2326274		97.1	0	0	0.862248	1.942	10	79%	53	106	0%	
Nitrobenzene-d5	S	ug/L	3.55873	69.1105366		97.1	0	0	1.015666	1.942	10	71%	55	111	0%	
Terphenyl-d14	S	ug/L	5.52609	107.316668		97.1	0	0	1.093346	1.942	10	111%	58	132	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14973252	B22010134-001	SVOC-8270-W-	SAMP	√5975.I\sh0110221/11/2022	2:09:0	1	162701	1/5/2022 8:0	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0206	0.1	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0176	0.1	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.0317	0.1	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.025	0.1	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.0283	0.1	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.0272	0.1	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.0347	0.1	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.0226	0.1	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.0267	0.1	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.0295	0.1	10	0%	0	0	0%	U
Chrysene	A	ug/L	0	0		0	0	0	0.0458	0.1	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.0367	0.1	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0	0		0	0	0	0.0233	0.1	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.0225	0.1	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.0491	0.1	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.029	0.1	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.0295	0.1	10	0%	0	0	0%	U
Pyrene	A	ug/L	0	0		0	0	0	0.0239	0.1	10	0%	0	0	0%	U
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
o-Terphenyl	X	ug/L	0	0		0	0	0	0.0654	0.1	10	0%	40	140	0%	U

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14973253	B22010134-001	SVOC-8270-W-	SAMP	√5975.I\sh0110221/11/2022	2:41:2	20	162701	1/5/2022 8:0	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
2-Fluorobiphenyl	S	ug/L	3.55104	71.0208		100	0	0	0.888	2	10	71%	53	106	0%	
Nitrobenzene-d5	S	ug/L	2.82308	56.4616		100	0	0	1.046	2	10	56%	55	111	0%	
Terphenyl-d14	S	ug/L	5.10523	102.1046		100	0	0	1.126	2	10	102%	58	132	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14973254	B22010141-001	SVOC-8270-W-	SAMP	√5975.I\sh0110221/11/2022	3:13:4	1	162701	1/5/2022 8:0	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.020806	0.101	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.017776	0.101	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.032017	0.101	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.02525	0.101	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.028583	0.101	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.027472	0.101	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.035047	0.101	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.022826	0.101	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.026967	0.101	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.029795	0.101	10	0%	0	0	0%	U
Chrysene	A	ug/L	0	0		0	0	0	0.046258	0.101	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.037067	0.101	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0	0		0	0	0	0.023533	0.101	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.022725	0.101	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.049591	0.101	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.02929	0.101	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.029795	0.101	10	0%	0	0	0%	U
Pyrene	A	ug/L	0	0		0	0	0	0.024139	0.101	10	0%	0	0	0%	U
1,4-Dichlorobenzene-d4	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%	0	0	0%	
Perylene-d12	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%	0	0	0%	
o-Terphenyl	X	ug/L	0	0		202	0	0	0.066054	0.101	10	0%	40	140	0%	US

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14973255	B22010141-001	SVOC-8270-W-	SAMP	√5975.I\sh0110221/11/2022	3:46:0	20	162701	1/5/2022 8:0	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
2-Fluorobiphenyl	S	ug/L	3.41794	69.042388		101	0	0	0.89688	2.02	10	68%	53	106	0%	
Nitrobenzene-d5	S	ug/L	3.09772	62.573944		101	0	0	1.05646	2.02	10	62%	55	111	0%	
Terphenyl-d14	S	ug/L	5.05837	102.179074		101	0	0	1.13726	2.02	10	101%	58	132	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14973256	B22010141-001	SVOC-8270-W-	MS-DOD	√5975.1\sh0110221/11/2022	4:18:3	1	162701	1/5/2022 8:0	1E+07	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	3.98071	4.0205171		5.05	0	0	0.020806	0.101	10	80%	41	115	0%	
2-Methylnaphthalene	A	ug/L	3.87022	3.9089222		5.05	0	0	0.017776	0.101	10	77%	39	114	0%	
Acenaphthene	A	ug/L	4.192	4.23392		5.05	0	0	0.032017	0.101	10	84%	48	114	0%	
Acenaphthylene	A	ug/L	4.44058	4.4849858		5.05	0	0	0.02525	0.101	10	89%	35	121	0%	
Anthracene	A	ug/L	5.09863	5.1496163		5.05	0	0	0.028583	0.101	10	102%	53	119	0%	
Benzo(a)anthracene	A	ug/L	5.0818	5.132618		5.05	0	0	0.027472	0.101	10	102%	59	120	0%	
Benzo(a)pyrene	A	ug/L	4.50962	4.5547162		5.05	0	0	0.035047	0.101	10	90%	53	120	0%	
Benzo(b)fluoranthene	A	ug/L	4.5194	4.564594		5.05	0	0	0.022826	0.101	10	90%	53	126	0%	
Benzo(g,h,i)perylene	A	ug/L	4.79401	4.8419501		5.05	0	0	0.026967	0.101	10	96%	44	128	0%	
Benzo(k)fluoranthene	A	ug/L	4.49154	4.5364554		5.05	0	0	0.029795	0.101	10	90%	54	125	0%	
Chrysene	A	ug/L	5.06512	5.1157712		5.05	0	0	0.046258	0.101	10	101%	57	120	0%	
Dibenzo(a,h)anthracene	A	ug/L	4.70789	4.7549689		5.05	0	0	0.037067	0.101	10	94%	44	141	0%	
Fluoranthene	A	ug/L	4.84154	4.8899554		5.05	0	0	0.023533	0.101	10	97%	58	120	0%	
Fluorene	A	ug/L	4.78964	4.8375364		5.05	0	0	0.022725	0.101	10	96%	50	118	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	4.62655	4.6728155		5.05	0	0	0.049591	0.101	10	93%	48	130	0%	
Naphthalene	A	ug/L	3.67164	3.7083564		5.05	0	0	0.02929	0.101	10	73%	43	114	0%	
Phenanthrene	A	ug/L	4.79762	4.8455962		5.05	0	0	0.029795	0.101	10	96%	53	115	0%	
Pyrene	A	ug/L	4.64179	4.6882079		5.05	0	0	0.024139	0.101	10	93%	53	121	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%			0%	
Acenaphthene-d10	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%			0%	
Chrysene-d12	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%			0%	
Naphthalene-d8	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%			0%	
Perylene-d12	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%			0%	
Phenanthrene-d10	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%			0%	
2-Fluorobiphenyl	S	ug/L	4.19602	4.2379802		5.05	0	0	0.044844	0.101	10	84%	53	106	0%	
Nitrobenzene-d5	S	ug/L	3.09677	3.1277377		5.05	0	0	0.052823	0.101	10	62%	55	111	0%	
Terphenyl-d14	S	ug/L	5.52315	5.5783815		5.05	0	0	0.056863	0.101	10	110%	58	132	0%	
o-Terphenyl	X	ug/L	4.27968	4.3224768		5.05	0	0	0.066054	0.101	10	86%	40	140	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14973257	B22010142-001	SVOC-8270-W-	SAMP	√5975.1\sh0110221/11/2022	4:50:5	1	162701	1/5/2022 8:0	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14973257	B22010142-001	SVOC-8270-W-	SAMP	√5975.I\sh0110221/11/2022	4:50:5	1	162701	1/5/2022 8:0	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.020188	0.1	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.017248	0.1	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.031066	0.1	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.0245	0.1	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.027734	0.1	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.026656	0.1	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.034006	0.1	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.022148	0.1	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.026166	0.1	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.02891	0.1	10	0%	0	0	0%	U
Chrysene	A	ug/L	0	0		0	0	0	0.044884	0.1	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.035966	0.1	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0	0		0	0	0	0.022834	0.1	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.02205	0.1	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.048118	0.1	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.02842	0.1	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.02891	0.1	10	0%	0	0	0%	U
Pyrene	A	ug/L	0	0		0	0	0	0.023422	0.1	10	0%	0	0	0%	U
1,4-Dichlorobenzene-d4	I	ug/L	40	39.2		0	0	0	0.098	0.1		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	39.2		0	0	0	0.098	0.1		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	39.2		0	0	0	0.098	0.1		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	39.2		0	0	0	0.098	0.1		0%	0	0	0%	
Perylene-d12	I	ug/L	40	39.2		0	0	0	0.098	0.1		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	39.2		0	0	0	0.098	0.1		0%	0	0	0%	
o-Terphenyl	X	ug/L	0	0		196	0	0	0.064092	0.1	10	0%	40	140	0%	US

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14973258	B22010142-001	SVOC-8270-W-	SAMP	√5975.I\sh0110221/11/2022	5:23:1	20	162701	1/5/2022 8:0	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
2-Fluorobiphenyl	S	ug/L	3.58978	70.359688		98	0	0	0.87024	1.96	10	72%	53	106	0%	
Nitrobenzene-d5	S	ug/L	2.85157	55.890772		98	0	0	1.02508	1.96	10	57%	55	111	0%	
Terphenyl-d14	S	ug/L	5.15255	100.98998		98	0	0	1.10348	1.96	10	103%	58	132	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14973259	B22010143-001	SVOC-8270-W-	SAMP	v5975.I\sh0110221/11/2022	5:55:2	1	162701	1/5/2022 8:0	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0196112	0.1	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0167552	0.1	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.0301784	0.1	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.0238	0.1	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.0269416	0.1	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.0258944	0.1	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.0330344	0.1	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.0215152	0.1	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.0254184	0.1	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.028084	0.1	10	0%	0	0	0%	U
Chrysene	A	ug/L	0	0		0	0	0	0.0436016	0.1	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.0349384	0.1	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0	0		0	0	0	0.0221816	0.1	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.02142	0.1	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.0467432	0.1	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.027608	0.1	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.028084	0.1	10	0%	0	0	0%	U
Pyrene	A	ug/L	0	0		0	0	0	0.0227528	0.1	10	0%	0	0	0%	U
1,4-Dichlorobenzene-d4	I	ug/L	40	38.08		0	0	0	0.0952	0.1		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	38.08		0	0	0	0.0952	0.1		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	38.08		0	0	0	0.0952	0.1		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	38.08		0	0	0	0.0952	0.1		0%	0	0	0%	
Perylene-d12	I	ug/L	40	38.08		0	0	0	0.0952	0.1		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	38.08		0	0	0	0.0952	0.1		0%	0	0	0%	
o-Terphenyl	X	ug/L	0	0		190.4	0	0	0.0622608	0.1	10	0%	40	140	0%	US

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14973260	B22010143-001	SVOC-8270-W-	SAMP	v5975.I\sh0110221/11/2022	6:27:5	20	162701	1/5/2022 8:0	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
2-Fluorobiphenyl	S	ug/L	3.54298	67.4583392		95.2	0	0	0.845376	1.904	10	71%	53	106	0%	
Nitrobenzene-d5	S	ug/L	2.84521	54.1727984		95.2	0	0	0.995792	1.904	10	57%	55	111	0%	
Terphenyl-d14	S	ug/L	5.19251	98.8653904		95.2	0	0	1.071952	1.904	10	104%	58	132	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14973261	B22010145-001	SVOC-8270-W-	SAMP	√5975.I\sh0110221/11/2022	7:00:0	1	162701	1/5/2022 8:0	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.020806	0.101	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.017776	0.101	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.032017	0.101	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.02525	0.101	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.028583	0.101	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.027472	0.101	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.035047	0.101	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.022826	0.101	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.026967	0.101	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.029795	0.101	10	0%	0	0	0%	U
Chrysene	A	ug/L	0	0		0	0	0	0.046258	0.101	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.037067	0.101	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0	0		0	0	0	0.023533	0.101	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.022725	0.101	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.049591	0.101	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.02929	0.101	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.029795	0.101	10	0%	0	0	0%	U
Pyrene	A	ug/L	0	0		0	0	0	0.024139	0.101	10	0%	0	0	0%	U
1,4-Dichlorobenzene-d4	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%	0	0	0%	
Perylene-d12	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%	0	0	0%	
o-Terphenyl	X	ug/L	0	0		202	0	0	0.066054	0.101	10	0%	40	140	0%	US

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14973262	B22010145-001	SVOC-8270-W-	SAMP	√5975.I\sh0110221/11/2022	7:32:2	20	162701	1/5/2022 8:0	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
2-Fluorobiphenyl	S	ug/L	3.65019	73.733838		101	0	0	0.89688	2.02	10	73%	53	106	0%	
Nitrobenzene-d5	S	ug/L	3.1253	63.13106		101	0	0	1.05646	2.02	10	63%	55	111	0%	
Terphenyl-d14	S	ug/L	5.48609	110.819018		101	0	0	1.13726	2.02	10	110%	58	132	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14973263	B22010148-001	SVOC-8270-W-	SAMP	√5975.I\sh0110221/11/2022	8:04:4	1	162701	1/5/2022 8:0	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.020394	0.1	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.017424	0.1	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.031383	0.1	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.02475	0.1	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.028017	0.1	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.026928	0.1	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.034353	0.1	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.022374	0.1	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.026433	0.1	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.029205	0.1	10	0%	0	0	0%	U
Chrysene	A	ug/L	0	0		0	0	0	0.045342	0.1	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.036333	0.1	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0	0		0	0	0	0.023067	0.1	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.022275	0.1	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.048609	0.1	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.02871	0.1	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.029205	0.1	10	0%	0	0	0%	U
Pyrene	A	ug/L	0	0		0	0	0	0.023661	0.1	10	0%	0	0	0%	U
1,4-Dichlorobenzene-d4	I	ug/L	40	39.6		0	0	0	0.099	0.1		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	39.6		0	0	0	0.099	0.1		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	39.6		0	0	0	0.099	0.1		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	39.6		0	0	0	0.099	0.1		0%	0	0	0%	
Perylene-d12	I	ug/L	40	39.6		0	0	0	0.099	0.1		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	39.6		0	0	0	0.099	0.1		0%	0	0	0%	
o-Terphenyl	X	ug/L	0	0		198	0	0	0.064746	0.1	10	0%	40	140	0%	US

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14973264	B22010148-001	SVOC-8270-W-	SAMP	√5975.I\sh0110221/11/2022	8:37:1	20	162701	1/5/2022 8:0	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
2-Fluorobiphenyl	S	ug/L	3.16	62.568		99	0	0	0.87912	1.98	10	63%	53	106	0%	
Nitrobenzene-d5	S	ug/L	2.73574	54.167652		99	0	0	1.03554	1.98	10	55%	55	111	0%	
Terphenyl-d14	S	ug/L	5.34864	105.903072		99	0	0	1.11474	1.98	10	107%	58	132	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14973265	B22010209-001	SVOC-8270-W-	SAMP	√5975.I\sh0110221/11/2022	9:09:3	1	162701	1/5/2022 1:1	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0198172	0.1	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0169312	0.1	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.0304954	0.1	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.02405	0.1	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.0272246	0.1	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.0261664	0.1	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.0333814	0.1	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.0217412	0.1	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.0256854	0.1	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.028379	0.1	10	0%	0	0	0%	U
Chrysene	A	ug/L	0	0		0	0	0	0.0440596	0.1	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.0353054	0.1	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0	0		0	0	0	0.0224146	0.1	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.021645	0.1	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.0472342	0.1	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.027898	0.1	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.028379	0.1	10	0%	0	0	0%	U
Pyrene	A	ug/L	0	0		0	0	0	0.0229918	0.1	10	0%	0	0	0%	U
1,4-Dichlorobenzene-d4	I	ug/L	40	38.48		0	0	0	0.0962	0.1		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	38.48		0	0	0	0.0962	0.1		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	38.48		0	0	0	0.0962	0.1		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	38.48		0	0	0	0.0962	0.1		0%	0	0	0%	
Perylene-d12	I	ug/L	40	38.48		0	0	0	0.0962	0.1		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	38.48		0	0	0	0.0962	0.1		0%	0	0	0%	
o-Terphenyl	X	ug/L	0	0		192.4	0	0	0.0629148	0.1	10	0%	40	140	0%	US

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14973266	B22010209-001	SVOC-8270-W-	SAMP	√5975.I\sh0110221/11/2022	9:42:0	20	162701	1/5/2022 1:1	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
2-Fluorobiphenyl	S	ug/L	2.76383	53.1760892		96.2	0	0	0.854256	1.924	10	55%	53	106	0%	
Nitrobenzene-d5	S	ug/L	2.41737	46.5101988		96.2	0	0	1.006252	1.924	10	48%	55	111	0%	S
Terphenyl-d14	S	ug/L	4.86352	93.5741248		96.2	0	0	1.083212	1.924	10	97%	58	132	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14973267	B22010211-001	SVOC-8270-W-	SAMP	√5975.I\sh0110221/11/2022	10:14:	1	162701	1/5/2022 1:1	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Acenaphthene	A	ug/L	0	0		0	0	0	0.033602	0.106	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.0265	0.106	10	0%	0	0	0%	U
Anthracene	A	ug/L	0.20041	0.2124346		0	0	0	0.029998	0.106	10	0%	0	0	0%	
Benzo(a)anthracene	A	ug/L	0.1524	0.161544		0	0	0	0.028832	0.106	10	0%	0	0	0%	
Benzo(a)pyrene	A	ug/L	0.08675	0.091955		0	0	0	0.036782	0.106	10	0%	0	0	0%	J
Benzo(b)fluoranthene	A	ug/L	0.14797	0.1568482		0	0	0	0.023956	0.106	10	0%	0	0	0%	
Benzo(g,h,i)perylene	A	ug/L	0.03944	0.0418064		0	0	0	0.028302	0.106	10	0%	0	0	0%	J
Benzo(k)fluoranthene	A	ug/L	0.04273	0.0452938		0	0	0	0.03127	0.106	10	0%	0	0	0%	J
Chrysene	A	ug/L	0.17315	0.183539		0	0	0	0.048548	0.106	10	0%	0	0	0%	
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.038902	0.106	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0.31535	0.334271		0	0	0	0.024698	0.106	10	0%	0	0	0%	
Fluorene	A	ug/L	0	0		0	0	0	0.02385	0.106	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0.06687	0.0708822		0	0	0	0.052046	0.106	10	0%	0	0	0%	J
Phenanthrene	A	ug/L	1.78104	1.8879024		0	0	0	0.03127	0.106	10	0%	0	0	0%	
Pyrene	A	ug/L	0.39365	0.417269		0	0	0	0.025334	0.106	10	0%	0	0	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	42.4		0	0	0	0.106	0.106		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	42.4		0	0	0	0.106	0.106		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	42.4		0	0	0	0.106	0.106		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	42.4		0	0	0	0.106	0.106		0%	0	0	0%	
Perylene-d12	I	ug/L	40	42.4		0	0	0	0.106	0.106		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	42.4		0	0	0	0.106	0.106		0%	0	0	0%	
o-Terphenyl	X	ug/L	0	0		212	0	0	0.069324	0.106	10	0%	40	140	0%	US

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14973268	B22010211-001	SVOC-8270-W-	SAMP	√5975.I\sh0110221/11/2022	10:46:	20	162701	1/5/2022 1:1	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Naphthalene	A	ug/L	5.99589	127.112868		0	0	0	0.6148	2.12	10	0%	0	0	0%	
2-Fluorobiphenyl	S	ug/L	3.4956	74.10672		106	0	0	0.94128	2.12	10	70%	53	106	0%	
Nitrobenzene-d5	S	ug/L	2.5982	55.08184		106	0	0	1.10876	2.12	10	52%	55	111	0%	S
Terphenyl-d14	S	ug/L	4.62492	98.048304		106	0	0	1.19356	2.12	10	92%	58	132	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14973269	10-Jan-22_CCV	SVOC-8270-W-	CCV	v5975.I\sh0110221/11/2022	11:19:	1	R372988		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	2.25355	2.25355		2	0	0	0.0206	0.1	10	113%	50	150	0%	
2-Methylnaphthalene	A	ug/L	1.96788	1.96788		2	0	0	0.0176	0.1	10	98%	50	150	0%	
Acenaphthene	A	ug/L	1.7267	1.7267		2	0	0	0.0317	0.1	10	86%	50	150	0%	
Acenaphthylene	A	ug/L	1.92677	1.92677		2	0	0	0.025	0.1	10	96%	50	150	0%	
Anthracene	A	ug/L	2.11507	2.11507		2	0	0	0.0283	0.1	10	106%	50	150	0%	
Benzo(a)anthracene	A	ug/L	1.91696	1.91696		2	0	0	0.0272	0.1	10	96%	50	150	0%	
Benzo(a)pyrene	A	ug/L	1.85533	1.85533		2	0	0	0.0347	0.1	10	93%	50	150	0%	
Benzo(b)fluoranthene	A	ug/L	1.79677	1.79677		2	0	0	0.0226	0.1	10	90%	50	150	0%	
Benzo(g,h,i)perylene	A	ug/L	2.03202	2.03202		2	0	0	0.0267	0.1	10	102%	50	150	0%	
Benzo(k)fluoranthene	A	ug/L	1.88438	1.88438		2	0	0	0.0295	0.1	10	94%	50	150	0%	
Chrysene	A	ug/L	2.06869	2.06869		2	0	0	0.0458	0.1	10	103%	50	150	0%	
Dibenzo(a,h)anthracene	A	ug/L	1.85632	1.85632		2	0	0	0.0367	0.1	10	93%	50	150	0%	
Fluoranthene	A	ug/L	1.88902	1.88902		2	0	0	0.0233	0.1	10	94%	50	150	0%	
Fluorene	A	ug/L	2.04572	2.04572		2	0	0	0.0225	0.1	10	102%	50	150	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	1.80099	1.80099		2	0	0	0.0491	0.1	10	90%	50	150	0%	
Naphthalene	A	ug/L	1.89087	1.89087		2	0	0	0.029	0.1	10	95%	50	150	0%	
Phenanthrene	A	ug/L	2.01698	2.01698		2	0	0	0.0295	0.1	10	101%	50	150	0%	
Pyrene	A	ug/L	1.9009	1.9009		2	0	0	0.0239	0.1	10	95%	50	150	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%	50	150	0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%	50	150	0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	50	150	0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%	50	150	0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	50	150	0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%	50	150	0%	
2-Fluorobiphenyl	S	ug/L	2.00267	2.00267		2	0	0	0.0444	0.1	10	100%	50	150	0%	
Nitrobenzene-d5	S	ug/L	1.72745	1.72745		2	0	0	0.0523	0.1	10	86%	50	150	0%	
Terphenyl-d14	S	ug/L	2.16726	2.16726		2	0	0	0.0563	0.1	10	108%	50	150	0%	
o-Terphenyl	X	ug/L	1.92307	1.92307		2	0	0	0.0654	0.1	10	96%	50	150	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976392	10-Jan-22_CCV	SVOC-8270C-SI	CCV	v5975.I\sh0110221/10/2022	11:59:	1	R372988		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976392	10-Jan-22_CC	SVOC-8270C-SI	CCV	v5975.I\sh0110221/10/2022	11:59:	1	R372988		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	2.35717	2.35717		2	0	0	0.0206	0.1	10	118%	80	120	0%	
2-Methylnaphthalene	A	ug/L	2.09598	2.09598		2	0	0	0.0176	0.1	10	105%	80	120	0%	
Acenaphthene	A	ug/L	1.71855	1.71855		2	0	0	0.0317	0.1	10	86%	80	120	0%	
Acenaphthylene	A	ug/L	1.92929	1.92929		2	0	0	0.025	0.1	10	96%	80	120	0%	
Anthracene	A	ug/L	2.05066	2.05066		2	0	0	0.0283	0.1	10	103%	80	120	0%	
Benzo(a)anthracene	A	ug/L	1.91912	1.91912		2	0	0	0.0272	0.1	10	96%	80	120	0%	
Benzo(a)pyrene	A	ug/L	1.88032	1.88032		2	0	0	0.0347	0.1	10	94%	80	120	0%	
Benzo(b)fluoranthene	A	ug/L	1.70536	1.70536		2	0	0	0.0226	0.1	10	85%	80	120	0%	
Benzo(g,h,i)perylene	A	ug/L	1.94311	1.94311		2	0	0	0.0267	0.1	10	97%	80	120	0%	
Benzo(k)fluoranthene	A	ug/L	1.99827	1.99827		2	0	0	0.0295	0.1	10	100%	80	120	0%	
Chrysene	A	ug/L	1.9925	1.9925		2	0	0	0.0458	0.1	10	100%	80	120	0%	
Dibenzo(a,h)anthracene	A	ug/L	1.79461	1.79461		2	0	0	0.0367	0.1	10	90%	80	120	0%	
Fluoranthene	A	ug/L	1.9127	1.9127		2	0	0	0.0233	0.1	10	96%	80	120	0%	
Fluorene	A	ug/L	2.01922	2.01922		2	0	0	0.0225	0.1	10	101%	80	120	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	1.68367	1.68367		2	0	0	0.0491	0.1	10	84%	80	120	0%	
Naphthalene	A	ug/L	1.93409	1.93409		2	0	0	0.029	0.1	10	97%	80	120	0%	
Phenanthrene	A	ug/L	2.00983	2.00983		2	0	0	0.0295	0.1	10	100%	80	120	0%	
Pyrene	A	ug/L	1.84756	1.84756		2	0	0	0.0239	0.1	10	92%	80	120	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1	10	0%	80	120	0%	
2-Fluorobiphenyl	S	ug/L	1.94547	1.94547		2	0	0	0.0444	0.1	10	97%	80	120	0%	
Nitrobenzene-d5	S	ug/L	1.7365	1.7365		2	0	0	0.0523	0.1	10	87%	80	120	0%	
Terphenyl-d14	S	ug/L	2.02994	2.02994		2	0	0	0.0563	0.1	10	101%	80	120	0%	
o-Terphenyl	X	ug/L	1.82838	1.82838		2	0	0	0.0654	0	0	91%	80	120	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976393	10-Jan-22_ISTB	SVOC-8270C-SI	SAMP	v5975.I\sh0110221/11/2022	12:31:	1	R372988		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976393	10-Jan-22_ISTB	SVOC-8270C-SI	SAMP	v5975.I\sh0110221/11/2022	12:31:	1	R372988		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0206	0.1	10	0%	0	0	0%	
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0176	0.1	10	0%	0	0	0%	
Acenaphthene	A	ug/L	0	0		0	0	0	0.0317	0.1	10	0%	0	0	0%	
Acenaphthylene	A	ug/L	0	0		0	0	0	0.025	0.1	10	0%	0	0	0%	
Anthracene	A	ug/L	0	0		0	0	0	0.0283	0.1	10	0%	0	0	0%	
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.0272	0.1	10	0%	0	0	0%	
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.0347	0.1	10	0%	0	0	0%	
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.0226	0.1	10	0%	0	0	0%	
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.0267	0.1	10	0%	0	0	0%	
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.0295	0.1	10	0%	0	0	0%	
Chrysene	A	ug/L	0	0		0	0	0	0.0458	0.1	10	0%	0	0	0%	
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.0367	0.1	10	0%	0	0	0%	
Fluoranthene	A	ug/L	0	0		0	0	0	0.0233	0.1	10	0%	0	0	0%	
Fluorene	A	ug/L	0	0		0	0	0	0.0225	0.1	10	0%	0	0	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.0491	0.1	10	0%	0	0	0%	
Naphthalene	A	ug/L	0	0		0	0	0	0.029	0.1	10	0%	0	0	0%	
Phenanthrene	A	ug/L	0	0		0	0	0	0.0295	0.1	10	0%	0	0	0%	
Pyrene	A	ug/L	0	0		0	0	0	0.0239	0.1	10	0%	0	0	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40000		0	0	0	0.1	0.1		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	40000		0	0	0	0.1	0.1		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	40000		0	0	0	0.1	0.1		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	40000		0	0	0	0.1	0.1		0%	0	0	0%	
Perylene-d12	I	ug/L	40	40000		0	0	0	0.1	0.1		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	40000		0	0	0	0.1	0.1	10	0%	0	0	0%	E
2-Fluorobiphenyl	S	ug/L	0	0		5	0	0	0.0444	0.1	10	0%	25	94	0%	S
Nitrobenzene-d5	S	ug/L	0	0		5	0	0	0.0523	0.1	10	0%	19	102	0%	S
Terphenyl-d14	S	ug/L	0	0		5	0	0	0.0563	0.1	10	0%	39	106	0%	S
o-Terphenyl	X	ug/L	0	0		200	0	0	0.0654	0	0	0%	40	140	0%	S

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976394	B22010120-001	SVOC-8270C-SI	SAMP	v5975.I\sh0110221/11/2022	1:04:1	1	162701	1/4/2022 3:4	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976394	B22010120-001	SVOC-8270C-SI	SAMP	√5975.I\sh0110221/11/2022	1:04:1	1	162701	1/4/2022 3:4	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0200026	0.1	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0170896	0.1	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.0307807	0.1	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.024275	0.1	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.0274793	0.1	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.0264112	0.1	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.0336937	0.1	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.0219446	0.1	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.0259257	0.1	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.0286445	0.1	10	0%	0	0	0%	U
Chrysene	A	ug/L	0	0		0	0	0	0.0444718	0.1	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.0356357	0.1	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0	0		0	0	0	0.0226243	0.1	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.0218475	0.1	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.0476761	0.1	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.028159	0.1	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.0286445	0.1	10	0%	0	0	0%	U
Pyrene	A	ug/L	0	0		0	0	0	0.0232069	0.1	10	0%	0	0	0%	U
1,4-Dichlorobenzene-d4	I	ug/L	40	38.84		0	0	0	0.0971	0.1		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	38.84		0	0	0	0.0971	0.1		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	38.84		0	0	0	0.0971	0.1		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	38.84		0	0	0	0.0971	0.1		0%	0	0	0%	
Perylene-d12	I	ug/L	40	38.84		0	0	0	0.0971	0.1		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	38.84		0	0	0	0.0971	0.1	10	0%	0	0	0%	E

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976395	B22010120-001	SVOC-8270C-SI	SAMP	√5975.I\sh0110221/11/2022	1:36:4	20	162701	1/4/2022 3:4	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976396	B22010134-001	SVOC-8270C-SI	SAMP	√5975.I\sh0110221/11/2022	2:09:0	1	162701	1/5/2022 8:0	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976396	B22010134-001	SVOC-8270C-SI	SAMP	√5975.I\sh0110221/11/2022	2:09:0	1	162701	1/5/2022 8:0	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0206	0.1	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0176	0.1	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.0317	0.1	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.025	0.1	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.0283	0.1	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.0272	0.1	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.0347	0.1	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.0226	0.1	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.0267	0.1	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.0295	0.1	10	0%	0	0	0%	U
Chrysene	A	ug/L	0	0		0	0	0	0.0458	0.1	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.0367	0.1	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0	0		0	0	0	0.0233	0.1	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.0225	0.1	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.0491	0.1	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.029	0.1	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.0295	0.1	10	0%	0	0	0%	U
Pyrene	A	ug/L	0	0		0	0	0	0.0239	0.1	10	0%	0	0	0%	U
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1	10	0%	0	0	0%	E
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976397	B22010134-001	SVOC-8270C-SI	SAMP	√5975.I\sh0110221/11/2022	2:41:2	20	162701	1/5/2022 8:0	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976398	B22010141-001	SVOC-8270C-SI	SAMP	√5975.I\sh0110221/11/2022	3:13:4	1	162701	1/5/2022 8:0	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976398	B22010141-001	SVOC-8270C-SI SAMP		√5975.I\sh0110221/11/2022	3:13:4	1	162701	1/5/2022 8:0	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.020806	0.101	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.017776	0.101	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.032017	0.101	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.02525	0.101	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.028583	0.101	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.027472	0.101	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.035047	0.101	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.022826	0.101	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.026967	0.101	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.029795	0.101	10	0%	0	0	0%	U
Chrysene	A	ug/L	0	0		0	0	0	0.046258	0.101	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.037067	0.101	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0	0		0	0	0	0.023533	0.101	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.022725	0.101	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.049591	0.101	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.02929	0.101	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.029795	0.101	10	0%	0	0	0%	U
Pyrene	A	ug/L	0	0		0	0	0	0.024139	0.101	10	0%	0	0	0%	U
1,4-Dichlorobenzene-d4	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%	0	0	0%	
Perylene-d12	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	40.4		0	0	0	0.101	0.101	10	0%	0	0	0%	E
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976399	B22010141-001	SVOC-8270C-SI SAMP		√5975.I\sh0110221/11/2022	3:46:0	20	162701	1/5/2022 8:0	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976400	B22010141-001	SVOC-8270C-SI MS-DOD		√5975.I\sh0110221/11/2022	4:18:3	1	162701	1/5/2022 8:0	1E+07	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976400	B22010141-001	SVOC-8270C-SI	MS-DOD	√5975.1\sh0110221/11/2022	4:18:3	1	162701	1/5/2022 8:0	1E+07	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	3.98071	4.0205171		5.05	0	0	0.020806	0.101	10	80%	41	115	0%	
2-Methylnaphthalene	A	ug/L	3.87022	3.9089222		5.05	0	0	0.017776	0.101	10	77%	39	114	0%	
Acenaphthene	A	ug/L	4.192	4.23392		5.05	0	0	0.032017	0.101	10	84%	48	114	0%	
Acenaphthylene	A	ug/L	4.44058	4.4849858		5.05	0	0	0.02525	0.101	10	89%	35	121	0%	
Anthracene	A	ug/L	5.09863	5.1496163		5.05	0	0	0.028583	0.101	10	102%	53	119	0%	
Benzo(a)anthracene	A	ug/L	5.0818	5.132618		5.05	0	0	0.027472	0.101	10	102%	59	120	0%	
Benzo(a)pyrene	A	ug/L	4.50962	4.5547162		5.05	0	0	0.035047	0.101	10	90%	53	120	0%	
Benzo(b)fluoranthene	A	ug/L	4.5194	4.564594		5.05	0	0	0.022826	0.101	10	90%	53	126	0%	
Benzo(g,h,i)perylene	A	ug/L	4.79401	4.8419501		5.05	0	0	0.026967	0.101	10	96%	44	128	0%	
Benzo(k)fluoranthene	A	ug/L	4.49154	4.5364554		5.05	0	0	0.029795	0.101	10	90%	54	125	0%	
Chrysene	A	ug/L	5.06512	5.1157712		5.05	0	0	0.046258	0.101	10	101%	57	120	0%	
Dibenzo(a,h)anthracene	A	ug/L	4.70789	4.7549689		5.05	0	0	0.037067	0.101	10	94%	44	141	0%	
Fluoranthene	A	ug/L	4.84154	4.8899554		5.05	0	0	0.023533	0.101	10	97%	58	120	0%	
Fluorene	A	ug/L	4.78964	4.8375364		5.05	0	0	0.022725	0.101	10	96%	50	118	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	4.62655	4.6728155		5.05	0	0	0.049591	0.101	10	93%	48	130	0%	
Naphthalene	A	ug/L	3.67164	3.7083564		5.05	0	0	0.02929	0.101	10	73%	43	114	0%	
Phenanthrene	A	ug/L	4.79762	4.8455962		5.05	0	0	0.029795	0.101	10	96%	53	115	0%	
Pyrene	A	ug/L	4.64179	4.6882079		5.05	0	0	0.024139	0.101	10	93%	53	121	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%			0%	
Acenaphthene-d10	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%			0%	
Chrysene-d12	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%			0%	
Naphthalene-d8	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%			0%	
Perylene-d12	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%			0%	
Phenanthrene-d10	I	ug/L	40	40.4		0	0	0	0.101	0.101	10	0%			0%	
2-Fluorobiphenyl	S	ug/L	4.19602	4.2379802		5.05	0	0	0.044844	0.101	10	84%	53	106	0%	
Nitrobenzene-d5	S	ug/L	3.09677	3.1277377		5.05	0	0	0.052823	0.101	10	62%	55	111	0%	
Terphenyl-d14	S	ug/L	5.52315	5.5783815		5.05	0	0	0.056863	0.101	10	110%	58	132	0%	
o-Terphenyl	X	ug/L	4.27968	4.3224768		5.05	0	0	0.066054	0	0	86%	40	140	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976401	B22010142-001	SVOC-8270C-SI	SAMP	√5975.1\sh0110221/11/2022	4:50:5	1	162701	1/5/2022 8:0	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976401	B22010142-001	SVOC-8270C-SI	SAMP	√5975.I\sh0110221/11/2022	4:50:5	1	162701	1/5/2022 8:0	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.020188	0.1	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.017248	0.1	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.031066	0.1	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.0245	0.1	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.027734	0.1	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.026656	0.1	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.034006	0.1	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.022148	0.1	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.026166	0.1	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.02891	0.1	10	0%	0	0	0%	U
Chrysene	A	ug/L	0	0		0	0	0	0.044884	0.1	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.035966	0.1	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0	0		0	0	0	0.022834	0.1	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.02205	0.1	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.048118	0.1	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.02842	0.1	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.02891	0.1	10	0%	0	0	0%	U
Pyrene	A	ug/L	0	0		0	0	0	0.023422	0.1	10	0%	0	0	0%	U
1,4-Dichlorobenzene-d4	I	ug/L	40	39.2		0	0	0	0.098	0.1		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	39.2		0	0	0	0.098	0.1		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	39.2		0	0	0	0.098	0.1		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	39.2		0	0	0	0.098	0.1		0%	0	0	0%	
Perylene-d12	I	ug/L	40	39.2		0	0	0	0.098	0.1		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	39.2		0	0	0	0.098	0.1	10	0%	0	0	0%	E

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976402	B22010142-001	SVOC-8270C-SI	SAMP	√5975.I\sh0110221/11/2022	5:23:1	20	162701	1/5/2022 8:0	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976403	B22010143-001	SVOC-8270C-SI	SAMP	√5975.I\sh0110221/11/2022	5:55:2	1	162701	1/5/2022 8:0	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976403	B22010143-001	SVOC-8270C-SI	SAMP	√5975.I\sh0110221/11/2022	5:55:2	1	162701	1/5/2022 8:0	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0196112	0.1	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0167552	0.1	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.0301784	0.1	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.0238	0.1	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.0269416	0.1	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.0258944	0.1	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.0330344	0.1	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.0215152	0.1	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.0254184	0.1	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.028084	0.1	10	0%	0	0	0%	U
Chrysene	A	ug/L	0	0		0	0	0	0.0436016	0.1	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.0349384	0.1	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0	0		0	0	0	0.0221816	0.1	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.02142	0.1	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.0467432	0.1	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.027608	0.1	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.028084	0.1	10	0%	0	0	0%	U
Pyrene	A	ug/L	0	0		0	0	0	0.0227528	0.1	10	0%	0	0	0%	U
1,4-Dichlorobenzene-d4	I	ug/L	40	38.08		0	0	0	0.0952	0.1		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	38.08		0	0	0	0.0952	0.1		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	38.08		0	0	0	0.0952	0.1		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	38.08		0	0	0	0.0952	0.1		0%	0	0	0%	
Perylene-d12	I	ug/L	40	38.08		0	0	0	0.0952	0.1		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	38.08		0	0	0	0.0952	0.1	10	0%	0	0	0%	E

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976404	B22010143-001	SVOC-8270C-SI	SAMP	√5975.I\sh0110221/11/2022	6:27:5	20	162701	1/5/2022 8:0	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976405	B22010145-001	SVOC-8270C-SI	SAMP	√5975.I\sh0110221/11/2022	7:00:0	1	162701	1/5/2022 8:0	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976405	B22010145-001	SVOC-8270C-SI	SAMP	√5975.I\sh0110221/11/2022	7:00:0	1	162701	1/5/2022 8:0	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.020806	0.101	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.017776	0.101	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.032017	0.101	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.02525	0.101	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.028583	0.101	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.027472	0.101	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.035047	0.101	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.022826	0.101	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.026967	0.101	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.029795	0.101	10	0%	0	0	0%	U
Chrysene	A	ug/L	0	0		0	0	0	0.046258	0.101	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.037067	0.101	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0	0		0	0	0	0.023533	0.101	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.022725	0.101	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.049591	0.101	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.02929	0.101	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.029795	0.101	10	0%	0	0	0%	U
Pyrene	A	ug/L	0	0		0	0	0	0.024139	0.101	10	0%	0	0	0%	U
1,4-Dichlorobenzene-d4	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%	0	0	0%	
Perylene-d12	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	40.4		0	0	0	0.101	0.101	10	0%	0	0	0%	E

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976406	B22010145-001	SVOC-8270C-SI	SAMP	√5975.I\sh0110221/11/2022	7:32:2	20	162701	1/5/2022 8:0	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976407	B22010148-001	SVOC-8270C-SI	SAMP	√5975.I\sh0110221/11/2022	8:04:4	1	162701	1/5/2022 8:0	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976407	B22010148-001	SVOC-8270C-SI	SAMP	√5975.I\sh0110221/11/2022	8:04:4	1	162701	1/5/2022 8:0	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.020394	0.1	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.017424	0.1	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.031383	0.1	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.02475	0.1	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.028017	0.1	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.026928	0.1	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.034353	0.1	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.022374	0.1	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.026433	0.1	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.029205	0.1	10	0%	0	0	0%	U
Chrysene	A	ug/L	0	0		0	0	0	0.045342	0.1	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.036333	0.1	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0	0		0	0	0	0.023067	0.1	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.022275	0.1	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.048609	0.1	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.02871	0.1	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.029205	0.1	10	0%	0	0	0%	U
Pyrene	A	ug/L	0	0		0	0	0	0.023661	0.1	10	0%	0	0	0%	U
1,4-Dichlorobenzene-d4	I	ug/L	40	39.6		0	0	0	0.099	0.1		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	39.6		0	0	0	0.099	0.1		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	39.6		0	0	0	0.099	0.1		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	39.6		0	0	0	0.099	0.1		0%	0	0	0%	
Perylene-d12	I	ug/L	40	39.6		0	0	0	0.099	0.1		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	39.6		0	0	0	0.099	0.1	10	0%	0	0	0%	E

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976408	B22010148-001	SVOC-8270C-SI	SAMP	√5975.I\sh0110221/11/2022	8:37:1	20	162701	1/5/2022 8:0	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976409	B22010209-001	SVOC-8270C-SI	SAMP	√5975.I\sh0110221/11/2022	9:09:3	1	162701	1/5/2022 1:1	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976409	B22010209-001	SVOC-8270C-SI	SAMP	√5975.I\sh0110221/11/2022	9:09:3	1	162701	1/5/2022 1:1	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0198172	0.1	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0169312	0.1	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.0304954	0.1	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.02405	0.1	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.0272246	0.1	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.0261664	0.1	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.0333814	0.1	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.0217412	0.1	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.0256854	0.1	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.028379	0.1	10	0%	0	0	0%	U
Chrysene	A	ug/L	0	0		0	0	0	0.0440596	0.1	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.0353054	0.1	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0	0		0	0	0	0.0224146	0.1	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.021645	0.1	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.0472342	0.1	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.027898	0.1	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.028379	0.1	10	0%	0	0	0%	U
Pyrene	A	ug/L	0	0		0	0	0	0.0229918	0.1	10	0%	0	0	0%	U
1,4-Dichlorobenzene-d4	I	ug/L	40	38.48		0	0	0	0.0962	0.1		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	38.48		0	0	0	0.0962	0.1		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	38.48		0	0	0	0.0962	0.1		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	38.48		0	0	0	0.0962	0.1		0%	0	0	0%	
Perylene-d12	I	ug/L	40	38.48		0	0	0	0.0962	0.1		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	38.48		0	0	0	0.0962	0.1	10	0%	0	0	0%	E

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976410	B22010209-001	SVOC-8270C-SI	SAMP	√5975.I\sh0110221/11/2022	9:42:0	20	162701	1/5/2022 1:1	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976411	B22010211-001	SVOC-8270C-SI	SAMP	√5975.I\sh0110221/11/2022	10:14:	1	162701	1/5/2022 1:1	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976411	B22010211-001	SVOC-8270C-SI	SAMP	√5975.I\sh0110221/11/2022	10:14:	1	162701	1/5/2022 1:1	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Acenaphthene	A	ug/L	0	0		0	0	0	0.033602	0.106	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.0265	0.106	10	0%	0	0	0%	U
Anthracene	A	ug/L	0.20041	0.2124346		0	0	0	0.029998	0.106	10	0%	0	0	0%	
Benzo(a)anthracene	A	ug/L	0.1524	0.161544		0	0	0	0.028832	0.106	10	0%	0	0	0%	
Benzo(a)pyrene	A	ug/L	0.08675	0.091955		0	0	0	0.036782	0.106	10	0%	0	0	0%	J
Benzo(b)fluoranthene	A	ug/L	0.14797	0.1568482		0	0	0	0.023956	0.106	10	0%	0	0	0%	
Benzo(g,h,i)perylene	A	ug/L	0.03944	0.0418064		0	0	0	0.028302	0.106	10	0%	0	0	0%	J
Benzo(k)fluoranthene	A	ug/L	0.04273	0.0452938		0	0	0	0.03127	0.106	10	0%	0	0	0%	J
Chrysene	A	ug/L	0.17315	0.183539		0	0	0	0.048548	0.106	10	0%	0	0	0%	
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.038902	0.106	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0.31535	0.334271		0	0	0	0.024698	0.106	10	0%	0	0	0%	
Fluorene	A	ug/L	0	0		0	0	0	0.02385	0.106	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0.06687	0.0708822		0	0	0	0.052046	0.106	10	0%	0	0	0%	J
Phenanthrene	A	ug/L	1.78104	1.8879024		0	0	0	0.03127	0.106	10	0%	0	0	0%	
Pyrene	A	ug/L	0.39365	0.417269		0	0	0	0.025334	0.106	10	0%	0	0	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	42.4		0	0	0	0.106	0.106		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	42.4		0	0	0	0.106	0.106		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	42.4		0	0	0	0.106	0.106		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	42.4		0	0	0	0.106	0.106		0%	0	0	0%	
Perylene-d12	I	ug/L	40	42.4		0	0	0	0.106	0.106		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	42.4		0	0	0	0.106	0.106	10	0%	0	0	0%	E



Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976412	B22010211-001	SVOC-8270C-SI	SAMP	√5975.I\sh0110221/11/2022	10:46:	20	162701	1/5/2022 1:1	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Naphthalene	A	ug/L	5.99589	127.112868		0	0	0	0.6148	2.12	10	0%	0	0	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976413	10-Jan-22_CC	SVOC-8270C-SI	CCV	√5975.I\sh0110221/11/2022	11:19:	1	R372988				0	0				
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	2.25355	2.25355		2	0	0	0.0206	0.1	10	113%	50	150	0%	
2-Methylnaphthalene	A	ug/L	1.96788	1.96788		2	0	0	0.0176	0.1	10	98%	50	150	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976413	10-Jan-22_CCV	SVOC-8270C-SI	CCV	V5975.I\sh0110221	11/2022 11:19:	1	R372988		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Acenaphthene	A	ug/L	1.7267	1.7267		2	0	0	0.0317	0.1	10	86%	50	150	0%	
Acenaphthylene	A	ug/L	1.92677	1.92677		2	0	0	0.025	0.1	10	96%	50	150	0%	
Anthracene	A	ug/L	2.11507	2.11507		2	0	0	0.0283	0.1	10	106%	50	150	0%	
Benzo(a)anthracene	A	ug/L	1.91696	1.91696		2	0	0	0.0272	0.1	10	96%	50	150	0%	
Benzo(a)pyrene	A	ug/L	1.85533	1.85533		2	0	0	0.0347	0.1	10	93%	50	150	0%	
Benzo(b)fluoranthene	A	ug/L	1.79677	1.79677		2	0	0	0.0226	0.1	10	90%	50	150	0%	
Benzo(g,h,i)perylene	A	ug/L	2.03202	2.03202		2	0	0	0.0267	0.1	10	102%	50	150	0%	
Benzo(k)fluoranthene	A	ug/L	1.88438	1.88438		2	0	0	0.0295	0.1	10	94%	50	150	0%	
Chrysene	A	ug/L	2.06869	2.06869		2	0	0	0.0458	0.1	10	103%	50	150	0%	
Dibenzo(a,h)anthracene	A	ug/L	1.85632	1.85632		2	0	0	0.0367	0.1	10	93%	50	150	0%	
Fluoranthene	A	ug/L	1.88902	1.88902		2	0	0	0.0233	0.1	10	94%	50	150	0%	
Fluorene	A	ug/L	2.04572	2.04572		2	0	0	0.0225	0.1	10	102%	50	150	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	1.80099	1.80099		2	0	0	0.0491	0.1	10	90%	50	150	0%	
Naphthalene	A	ug/L	1.89087	1.89087		2	0	0	0.029	0.1	10	95%	50	150	0%	
Phenanthrene	A	ug/L	2.01698	2.01698		2	0	0	0.0295	0.1	10	101%	50	150	0%	
Pyrene	A	ug/L	1.9009	1.9009		2	0	0	0.0239	0.1	10	95%	50	150	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%	50	150	0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%	50	150	0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	50	150	0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%	50	150	0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	50	150	0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1	10	0%	50	150	0%	
2-Fluorobiphenyl	S	ug/L	2.00267	2.00267		2	0	0	0.0444	0.1	10	100%	50	150	0%	
Nitrobenzene-d5	S	ug/L	1.72745	1.72745		2	0	0	0.0523	0.1	10	86%	50	150	0%	
Terphenyl-d14	S	ug/L	2.16726	2.16726		2	0	0	0.0563	0.1	10	108%	50	150	0%	
o-Terphenyl	X	ug/L	1.92307	1.92307		2	0	0	0.0654	0	0	96%	50	150	0%	






Tune Evaluation Report

Data Path: \\MASSHUNTER\Org\Data\SV5975.I\sh011022\2 e8270d bna SIM\Jan1024.D
 Acq on: 1/10/2022 11:36:00 PM
 Operator: LIMS import
 Sample: 10-Jan-22_TUNE_24
 Inst Name: GCMS
 ALS Vial: 24
 Method: \\MASSHUNTER\Org\Data\SV5975.I\Methods\DFTPP5975625.m




Target Mass	Rel. To Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Pass/Fail
51	198	30	60	51.3	147008	Pass
68	69	0	2	0.0	0	Pass
70	69	0	2	0.4	977	Pass
127	198	40	60	54.8	157056	Pass
197	198	0	1	0.0	0	Pass
198	198	100	100	100.0	286464	Pass
199	198	5	9	6.7	19256	Pass
275	198	10	30	28.9	82872	Pass
365	198	1	100	3.2	9148	Pass
441	443	1E-10	150	93.6	32576	Pass
442	198	40	100	64.7	185280	Pass
443	442	17	23	18.8	34792	Pass
69	69	100	100	100.0	235008	Pass

Tune Evaluation Report



Tune Evaluation Report


+ Scan (rt: 8.180-8.220 min, 28 scans) Jan1024.D 4,4'-DDE




Compound Name	Expected RT	Observed RT	TIC Area	Breakdown %	Pass/Fail
4,4'-DDT	8.800	8.723	3774911	4.8	Pass
4,4'-DDD	8.500	8.423	192099		
4,4'-DDE	8.200	0.000	0		

Tune Evaluation Report

+ Scan (rt: 6.420 min) Jan1024.D Pentachlorophenol



+ Scan (rt: 7.953 min) Jan1024.D Benzidine




Compound Name	Expected RT	Observed RT	Tailing Factor	PGF	Pass/Fail
Pentachlorophenol	6.800	6.420	0.5	3.7	Pass
Benzidine	8.400	7.953	0.2	2.3	Pass

Quantitation Results Report (QT Reviewed)

Data File	Jan1025.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/10/2022 11:59:38 PM
Sample Name	10-Jan-22_CCV_25	Instrument	GCMS
Vial	25	Multiplier	1.00
DA Method File	011022 bna SIM 1.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 2.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	224889	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	419423	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	262799	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.792	188.0	554012	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	439231	40.0000	ng/ml	-0.013
M Perylene-d12	18.512	264.0	309386	40.0000	ng/ml	-0.013
System Monitoring Compounds						
S Nitrobenzene-d5	5.156	82.0	8991	1.7365	ng/ml	-0.013
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 34.73%		
S 2-Fluorobiphenyl	7.264	172.0	25453	1.9455	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 38.91%		
S o-Terphenyl	10.324	230.0	18573	1.8284	ng/ml	0.000
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = 36.57%		*
S Terphenyl-d14	12.288	244.0	16498	2.0299	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 40.60%		
Target Compounds						
T Naphthalene	5.966	128.0	27239	1.9341	ng/ml	99
T 2-Methylnaphthalene	6.790	141.0	17024	2.0960	ng/ml	91
T 1-Methylnaphthalene	6.902	141.0	17703	2.3572	ng/ml	94
T Acenaphthylene	7.838	152.0	27115	1.9293	ng/ml	100
T Acenaphthene	8.050	154.0	17560	1.7185	ng/ml	98
T Fluorene	8.673	166.0	23611	2.0192	ng/ml	97
T Phenanthrene	9.817	178.0	33791	2.0098	ng/ml	91
T Anthracene	9.879	178.0	27562	2.0507	ng/ml	94
T Fluoranthene	11.435	202.0	36121	1.9127	ng/ml	98
T Pyrene	11.806	202.0	40482	1.8476	ng/ml	97
T Benzo(a)Anthracene	14.726	228.0	25589	1.9191	ng/ml	100
T Chrysene	14.813	228.0	35970	1.9925	ng/ml	99
T Benzo(b)fluoranthene	17.745	252.0	22749	1.7054	ng/ml	98


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	17.820	252.0	27176	1.9983	ng/ml	92
T Benzo(a)pyrene	18.400	252.0	17510	1.8803	ng/ml	98
T Indeno(1,2,3-cd)pyrene	20.254	276.0	15598	1.6837	ng/ml	96
T Dibenzo(a,h)anthracene	20.315	278.0	19314	1.7946	ng/ml	97
T Benzo(g,h,i)perylene	20.575	276.0	25659	1.9431	ng/ml	93


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	1.7365	5.16	-0.01	8991	54.0	32.8	21.6	40.2
					128.0	35.9	21.3	39.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	1.9341	5.97	-0.01	27239	102.0	16.2	0.0	46.6
					129.0	11.1	7.6	14.1






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	2.0960	6.79	-0.01	17024	142.0	135.7	103.3	191.8
					115.0	59.2	36.8	68.3






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	2.3572	6.90	0.00	17703	142.0	116.8	77.9	144.7
					115.0	57.6	44.4	82.5






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	1.9455	7.26	0.00	25453	171.0	36.1	26.4	49.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthylene	1.9293	7.84	0.00	27115	153.0	14.6	10.2	18.9






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	1.7185	8.05	0.00	17560	153.0	112.4	80.3	149.2
					152.0	52.9	38.4	71.4






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene	2.0192	8.67	-0.01	23611	165.0	99.7	67.5	125.3
					167.0	12.7	7.9	14.6






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Phenanthrene	2.0098	9.82	0.00	33791	176.0	19.2	10.9	20.2



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Anthracene	2.0507	9.88	0.00	27562	176.0	19.2	11.6	21.6




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
o-Terphenyl	1.8284	10.32	0.00	18573	229.0	68.7	46.7	86.8
					215.0	44.0	30.2	56.2




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
----------	-------	----	----------	-------	------	--------	-------	-------




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
----------	-------	----	----------	-------	------	--------	-------	-------



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
----------	-------	----	----------	-------	------	--------	-------	-------




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
----------	-------	----	----------	-------	------	--------	-------	-------




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	1.9925	14.81	-0.01	35970	226.0	31.3	22.2	41.2
					229.0	21.8	15.5	28.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(b)fluoranthene	1.7054	17.75	-0.01	22749	253.0	21.9	15.8	29.4












Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(k)fluoranthene	1.9983	17.82	0.00	27176	253.0	19.2	16.1	30.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene	1.8803	18.40	0.00	17510	253.0	24.8	16.6	30.8




Quantitation Results Report (QT Reviewed)

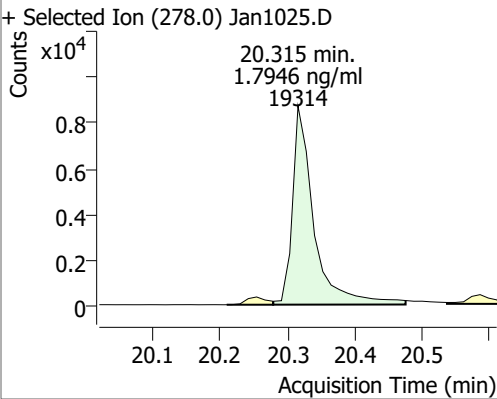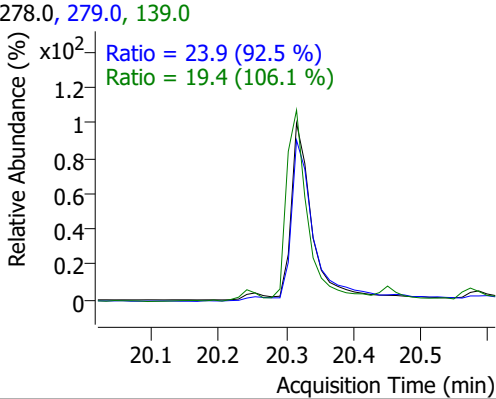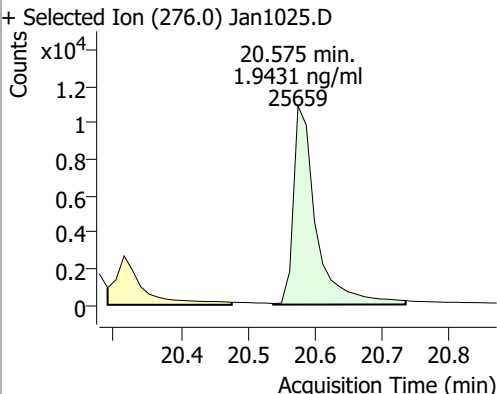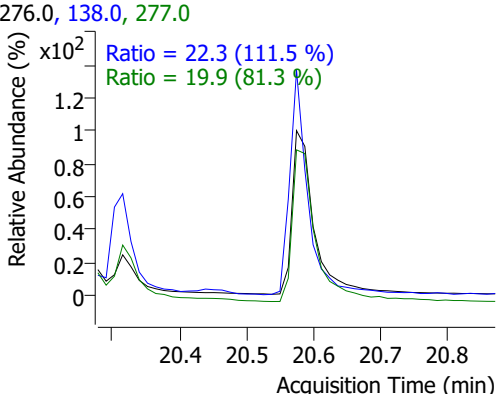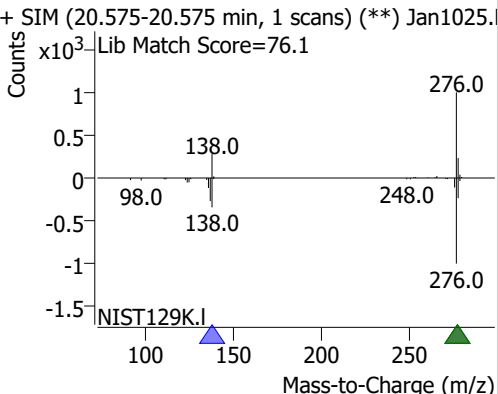Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Indeno(1,2,3-cd)pyrene	1.6837	20.25	0.01	15598	138.0	27.3	17.6	32.7
+ Selected Ion (276.0) Jan1025.D			276.0, 138.0			+ SIM (20.254-20.254 min, 1 scans) (**) Jan1025. Lib Match Score=76.0		
								
Dibenzo(a,h)anthracene	1.7946	20.32	0.00	19314	279.0	23.9	18.1	33.6
+ Selected Ion (278.0) Jan1025.D			278.0, 279.0, 139.0			+ SIM (20.315-20.315 min, 1 scans) (**) Jan1025. Lib Match Score=75.3		
								
Benzo(g,h,i)perylene	1.9431	20.57	0.00	25659	277.0	19.9	17.1	31.8
+ Selected Ion (276.0) Jan1025.D			276.0, 138.0, 277.0			+ SIM (20.575-20.575 min, 1 scans) (**) Jan1025. Lib Match Score=76.1		
								

Quantitation Results Report (QT Reviewed)

Data File	Jan1026.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/11/2022 12:31:55 AM
Sample Name	10-Jan-22_ISTBLK_26	Instrument	GCMS
Vial	26	Multiplier	1.00
DA Method File	011022 bna SIM 1.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 2.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)	QValue
Internal Standards							
M 1,4-Dichlorobenzene-d4	4.522	152.0	207630	40.0000	ng/ml	-0.025	
M Naphthalene-d8	5.941	136.0	408962	40.0000	ng/ml	-0.013	
M Acenaphthene-d10	8.013	164.0	258937	40.0000	ng/ml	0.000	
M Phenanthrene-d10	9.793	188.0	551100	40.0000	ng/ml	0.000	
M Chrysene-d12	14.751	240.0	434001	40.0000	ng/ml	-0.013	
M Perylene-d12	18.512	264.0	306940	40.0000	ng/ml	-0.013	
System Monitoring Compounds							
S Nitrobenzene-d5	0.000		0	N.D.			
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = NA%			
S 2-Fluorobiphenyl	0.000		0	N.D.			
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = NA%			
S o-Terphenyl	0.000		0	N.D.			
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%			
S Terphenyl-d14	0.000		0	N.D.			
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = NA%			
Target Compounds							
T Naphthalene	0.000		0	N.D.			
T 2-Methylnaphthalene	0.000		0	N.D.			
T 1-Methylnaphthalene	0.000		0	N.D.			
T Acenaphthylene	0.000		0	N.D.			
T Acenaphthene	8.050	154.0	0		ng/ml	md	1
T Fluorene	0.000		0	N.D.			
T Phenanthrene	0.000		0	N.D.			
T Anthracene	0.000		0	N.D.			
T Fluoranthene	0.000		0	N.D.			
T Pyrene	0.000		0	N.D.			
T Benzo(a)Anthracene	14.751	228.0	0		ng/ml	md	1
T Chrysene	14.751	228.0	0		ng/ml	md	1
T Benzo(b)fluoranthene	0.000		0	N.D.			


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.400	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Nitrobenzene-d5	N.D.	5.17	54.0	30.9	128.0	30.4




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
2-Fluorobiphenyl	N.D.	7.26	171.0	37.7




Compound	Conc.	Exp RT	QIon	Exp Ratio
Acenaphthylene	N.D.	7.84	153.0	14.6



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene		0		0	153.0		80.3	149.2
					152.0		38.4	71.4




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Fluorene	N.D.	8.69	165.0	96.4	167.0	11.3




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Phenanthrene	N.D.	9.82	176.0	15.5




Compound	Conc.	Exp RT	QIon	Exp Ratio
Anthracene	N.D.	9.88	176.0	16.6



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
o-Terphenyl	N.D.	10.32	229.0	66.8	215.0	43.2




Compound	Conc.	Exp RT	QIon	Exp Ratio
Fluoranthene	N.D.	11.44	101.0	11.4




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Pyrene	N.D.	11.82	101.0	13.9




Compound	Conc.	Exp RT	QIon	Exp Ratio
Terphenyl-d14	N.D.	12.29	122.0	13.7



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)Anthracene		0		0	226.0		19.5	36.3
					229.0		16.5	30.6




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene		0		0	226.0		22.2	41.2
					229.0		15.5	28.9




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.6	30.8




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1027.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/11/2022 1:04:19 AM
Sample Name	B22010120-001C	Instrument	GCMS
Vial	27	Multiplier	1.00
DA Method File	011022 bna SIM 1.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 2.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	244266	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	450555	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	265899	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.780	188.0	548178	40.0000	ng/ml	-0.013
M Chrysene-d12	14.751	240.0	443898	40.0000	ng/ml	-0.013
M Perylene-d12	18.512	264.0	334467	40.0000	ng/ml	-0.013
System Monitoring Compounds						
S Nitrobenzene-d5	5.143	82.0	536962	44.8566	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 897.13%		*
S 2-Fluorobiphenyl	7.264	172.0	991136	74.8723	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1497.45%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.288	244.0	923282	112.4061	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 2248.12%		*
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.013	154.0	0		ng/ml	md 1
T Fluorene	8.985	166.0	0		ng/ml	md 1
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.751	228.0	0		ng/ml	md 1
T Chrysene	14.751	228.0	0		ng/ml	md 1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.512	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	44.8566	5.14	-0.03	536962	54.0	34.1	21.6	40.2
					128.0	32.7	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5











Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4







Quantitation Results Report (QT Reviewed)



Quantitation Results Report (QT Reviewed)

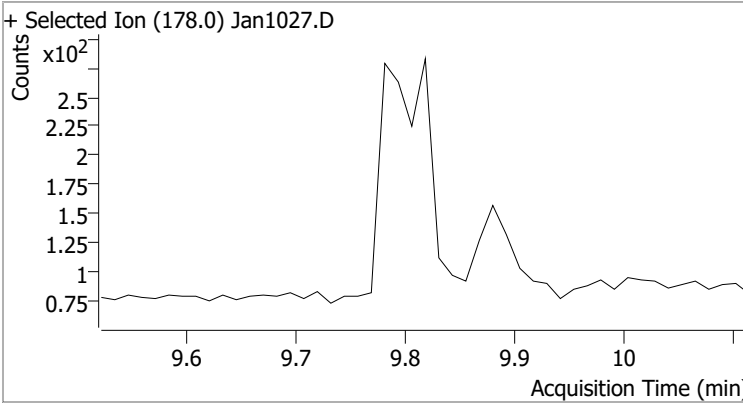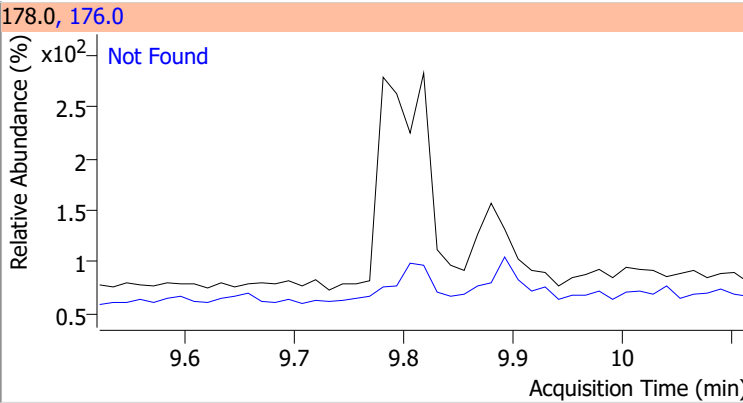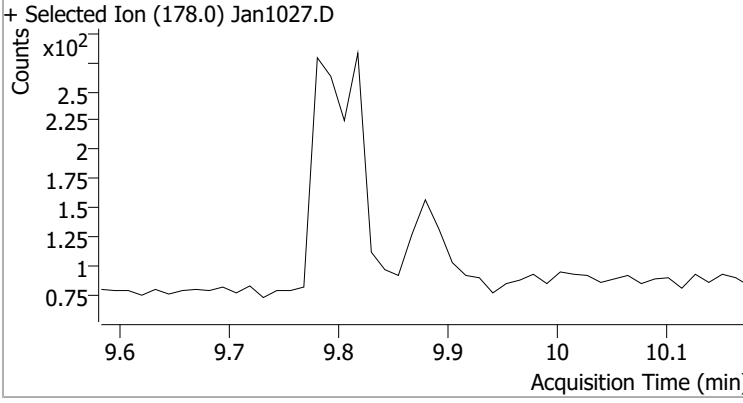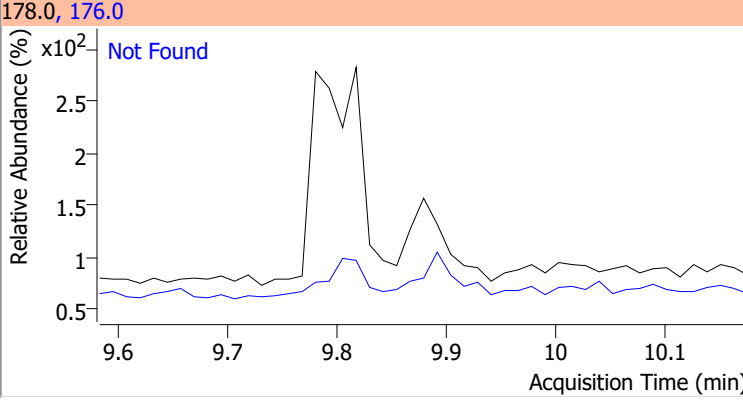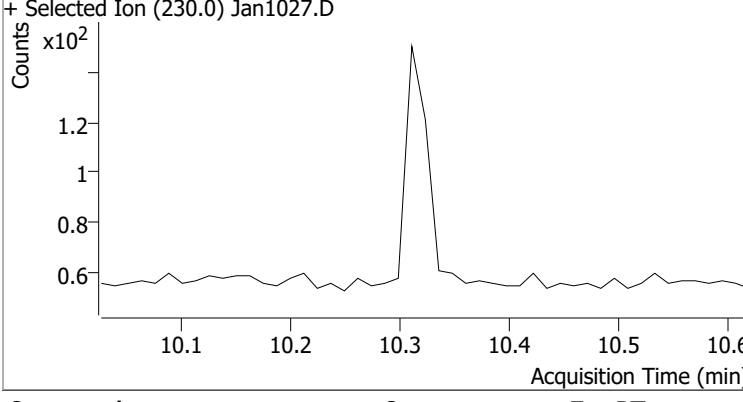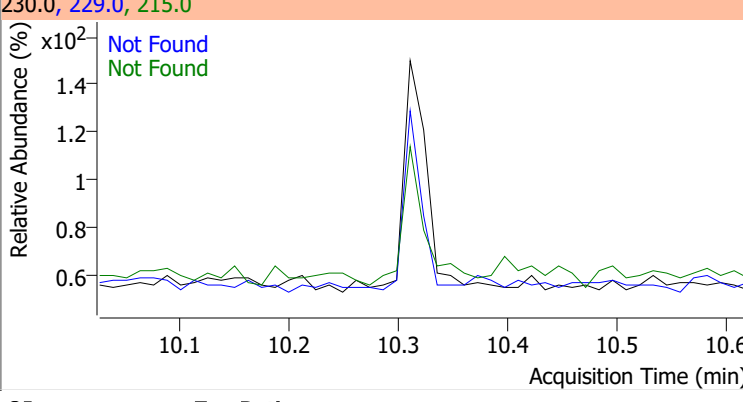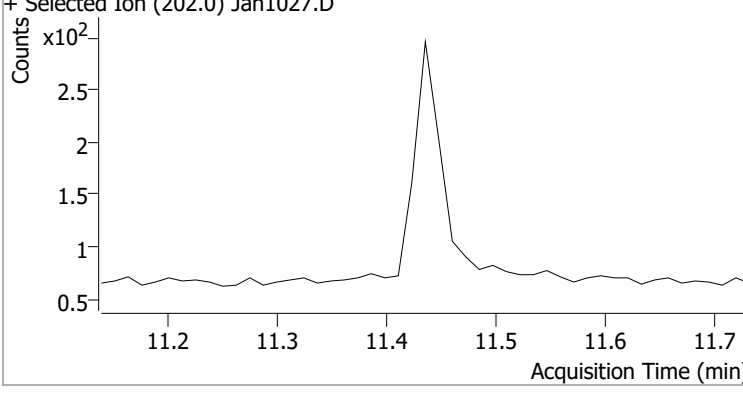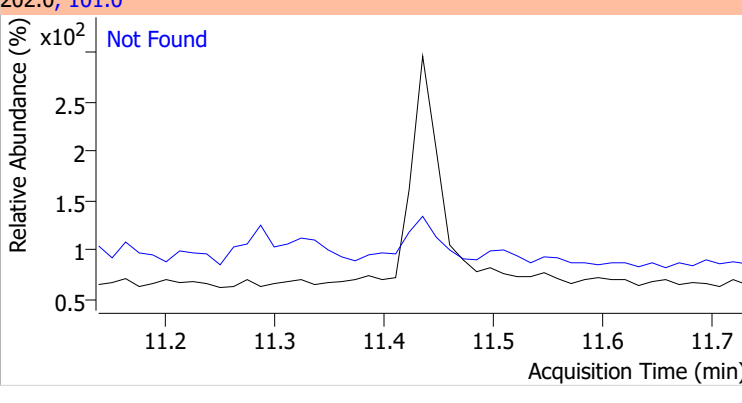
Compound	Conc.	Exp RT	QIon	Exp Ratio		
Phenanthrene	N.D.	9.82	176.0	15.5		
+ Selected Ion (178.0) Jan1027.D 			178.0, 176.0 			
Anthracene	N.D.	9.88	176.0	16.6		
+ Selected Ion (178.0) Jan1027.D 			178.0, 176.0 			
o-Terphenyl	N.D.	10.32	229.0	66.8	QIon	Exp Ratio
			215.0	43.2		
+ Selected Ion (230.0) Jan1027.D 			230.0, 229.0, 215.0 			
Fluoranthene	N.D.	11.44	101.0	11.4		
+ Selected Ion (202.0) Jan1027.D 			202.0, 101.0 			

Quantitation Results Report (QT Reviewed)

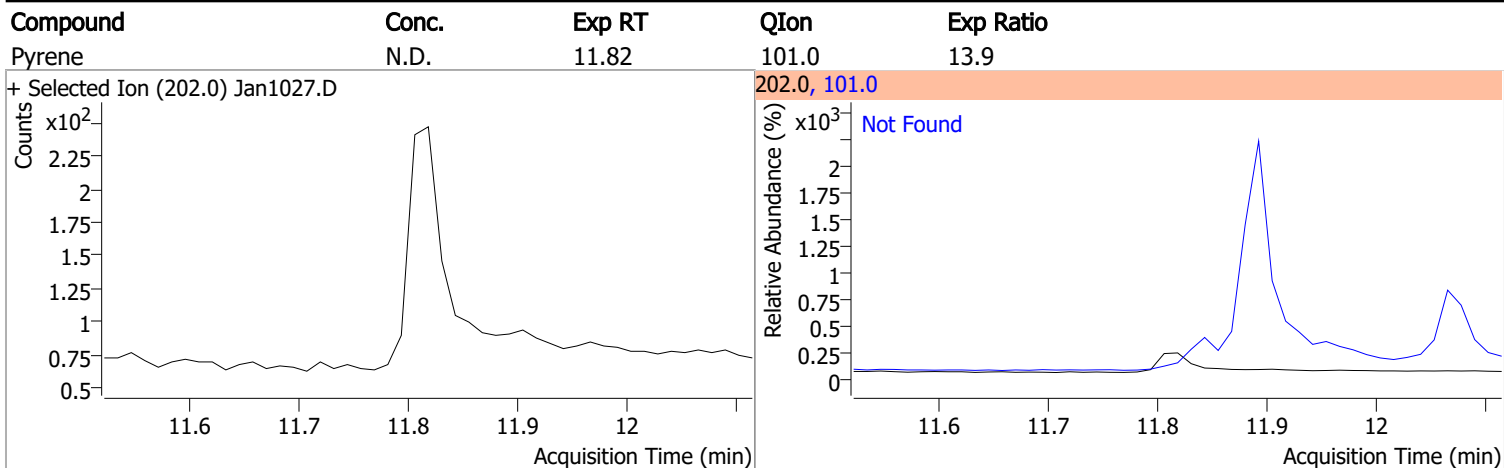


Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.6	30.8





Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2





Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1028.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/11/2022 1:36:40 AM
Sample Name	B22010120-001C	Instrument	GCMS
Vial	28	Multiplier	20.00
DA Method File	011022 bna SIM 1.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 2.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	243233	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	448051	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	273336	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.793	188.0	573742	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	465233	40.0000	ng/ml	-0.013
M Perylene-d12	18.524	264.0	349081	40.0000	ng/ml	0.000
System Monitoring Compounds						
S Nitrobenzene-d5	5.156	82.0	20988	71.1746	ng/ml	-0.013
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 1423.49% *		
S 2-Fluorobiphenyl	7.264	172.0	53418	78.5094	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1570.19% *		
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.275	244.0	47572	110.5218	ng/ml	-0.013
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 2210.44% *		
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.013	154.0	0		ng/ml md	1
T Fluorene	0.000		0	N.D.		
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.751	228.0	0		ng/ml md	1
T Chrysene	14.751	228.0	0		ng/ml md	1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.400	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	71.1746	5.16	-0.01	20988	54.0	28.0	21.6	40.2
					128.0	33.0	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	78.5094	7.26	0.00	53418	171.0	36.4	26.4	49.0




Compound	Conc.	Exp RT	QIon	Exp Ratio
Acenaphthylene	N.D.	7.84	153.0	14.6



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene		0		0	153.0		80.3	149.2
					152.0		38.4	71.4




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Fluorene	N.D.	8.69	165.0	96.4	167.0	11.3




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Phenanthrene	N.D.	9.82	176.0	15.5




Compound	Conc.	Exp RT	QIon	Exp Ratio
Anthracene	N.D.	9.88	176.0	16.6







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
o-Terphenyl	N.D.	10.32	229.0	66.8	215.0	43.2



Compound	Conc.	Exp RT	QIon	Exp Ratio
Fluoranthene	N.D.	11.44	101.0	11.4




Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.6	30.8




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1029.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/11/2022 2:09:04 AM
Sample Name	B22010134-001C	Instrument	GCMS
Vial	29	Multiplier	1.00
DA Method File	011022 bna SIM 1.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 2.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	261111	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	459520	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	270922	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.793	188.0	586610	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	452599	40.0000	ng/ml	-0.012
M Perylene-d12	18.524	264.0	342741	40.0000	ng/ml	0.000
System Monitoring Compounds						
S Nitrobenzene-d5	5.143	82.0	487628	40.3306	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 806.61%		*
S 2-Fluorobiphenyl	7.265	172.0	904677	67.0739	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1341.48%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.288	244.0	917206	109.5198	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 2190.40%		*
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.013	154.0	0		ng/ml	md
T Fluorene	0.000		0	N.D.		
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.751	228.0	0		ng/ml	md
T Chrysene	14.751	228.0	0		ng/ml	md
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.512	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	40.3306	5.14	-0.02	487628	54.0	34.2	21.6	40.2
					128.0	32.2	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	67.0739	7.26	0.00	904677	171.0	39.5	26.4	49.0




Compound	Conc.	Exp RT	QIon	Exp Ratio
Acenaphthylene	N.D.	7.84	153.0	14.6







Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene		0		0	153.0		80.3	149.2
					152.0		38.4	71.4







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Fluorene	N.D.	8.69	165.0	96.4	167.0	11.3



Quantitation Results Report (QT Reviewed)

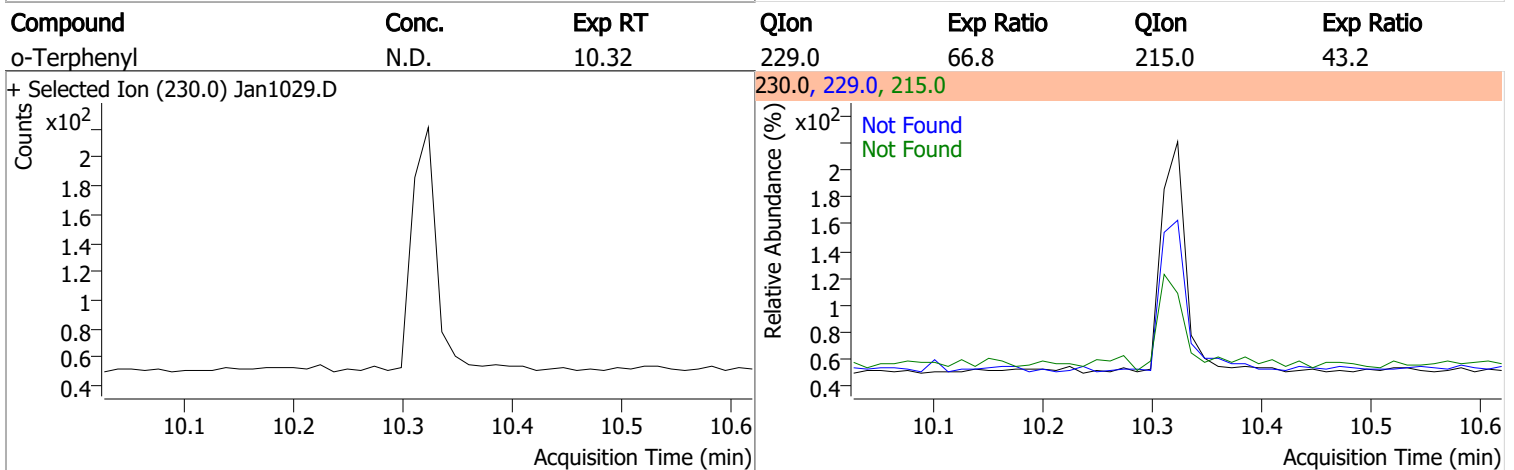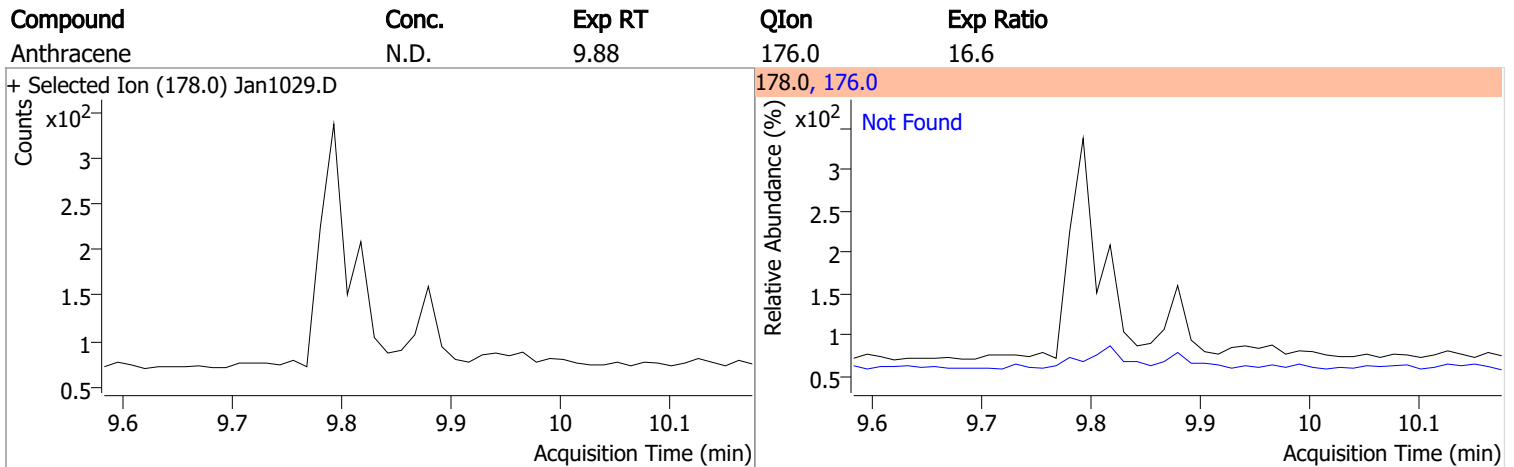


Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.6	30.8




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1030.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/11/2022 2:41:23 AM
Sample Name	B22010134-001C	Instrument	GCMS
Vial	30	Multiplier	20.00
DA Method File	011022 bna SIM 1.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 2.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	224965	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	420396	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	255779	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.793	188.0	538555	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	427477	40.0000	ng/ml	-0.013
M Perylene-d12	18.512	264.0	317090	40.0000	ng/ml	-0.012
System Monitoring Compounds						
S Nitrobenzene-d5	5.156	82.0	15099	56.4617	ng/ml	-0.013
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 1129.23%		*
S 2-Fluorobiphenyl	7.265	172.0	45219	71.0207	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1420.41%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.288	244.0	40382	102.1046	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 2042.09%		*
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.050	154.0	0		ng/ml md	1
T Fluorene	0.000		0	N.D.		
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.751	228.0	0		ng/ml md	1
T Chrysene	14.814	228.0	0		ng/ml md	1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.413	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	56.4617	5.16	-0.01	15099	54.0	35.6	21.6	40.2
					128.0	36.4	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	71.0207	7.26	0.00	45219	171.0	35.6	26.4	49.0




Compound	Conc.	Exp RT	QIon	Exp Ratio
Acenaphthylene	N.D.	7.84	153.0	14.6











Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene		0		0	153.0		80.3	149.2
					152.0		38.4	71.4







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Fluorene	N.D.	8.69	165.0	96.4	167.0	11.3



Quantitation Results Report (QT Reviewed)

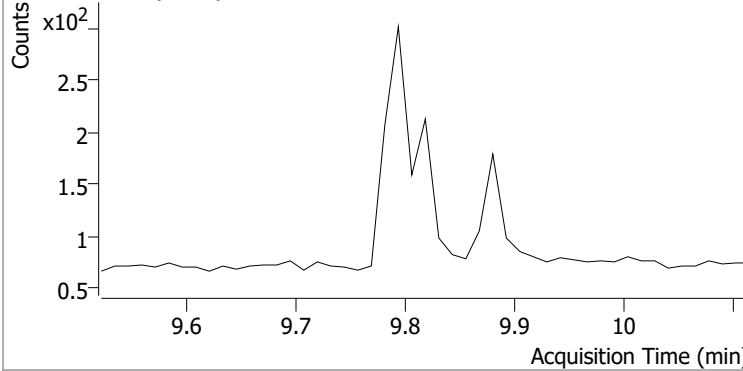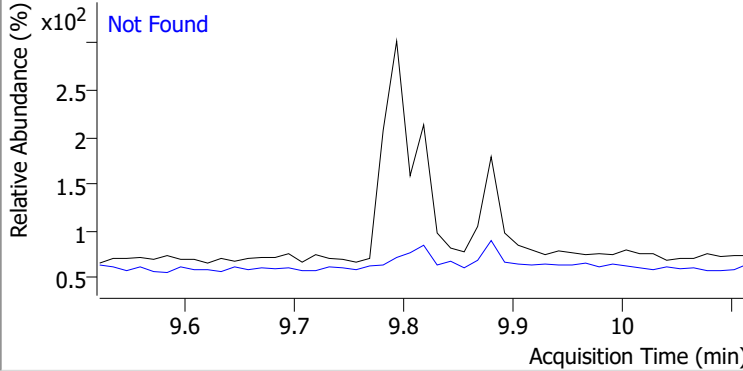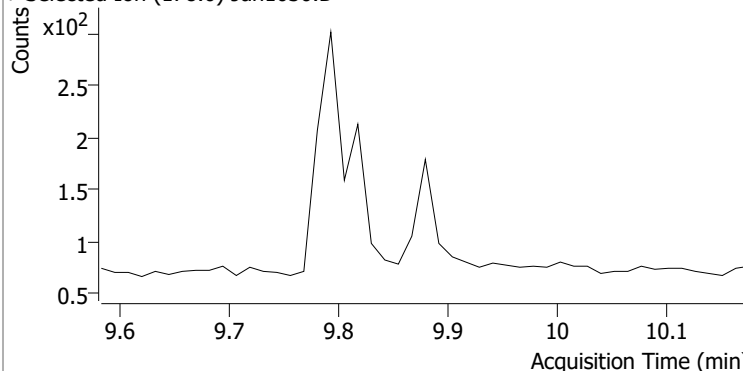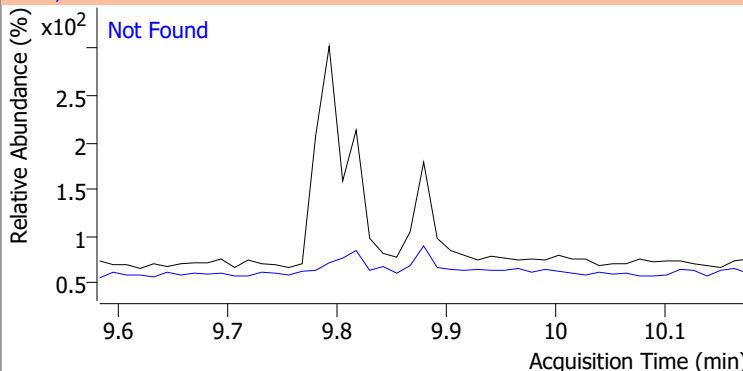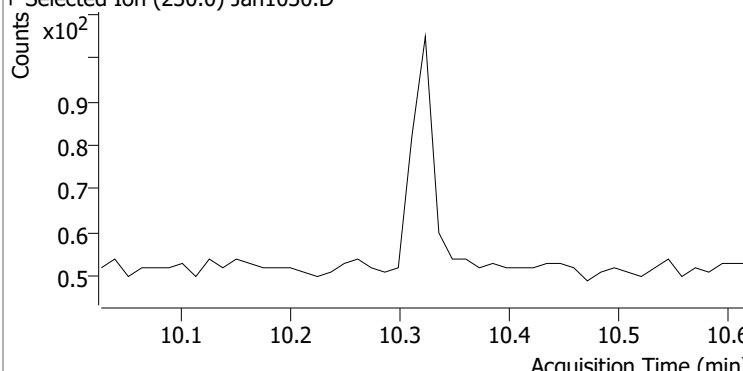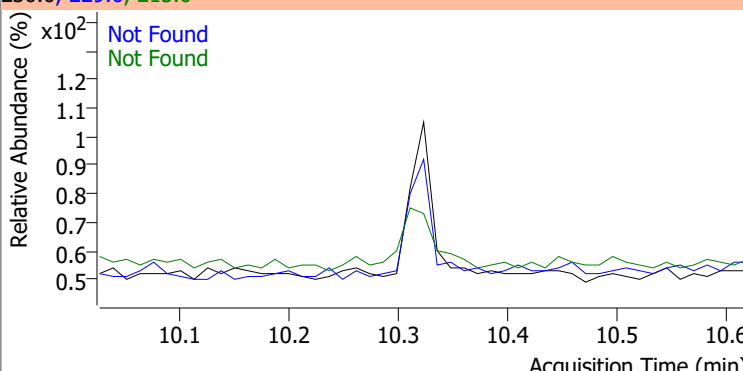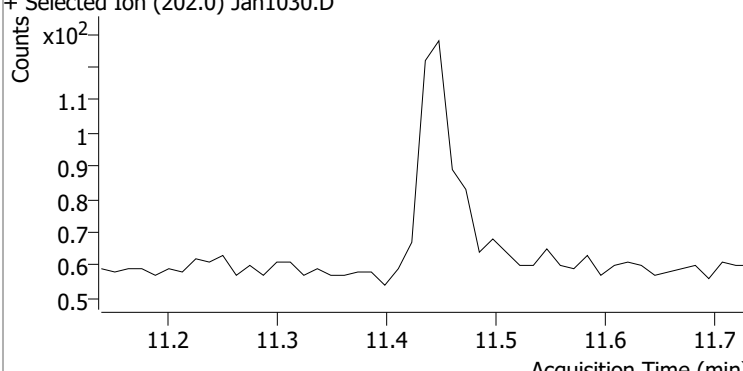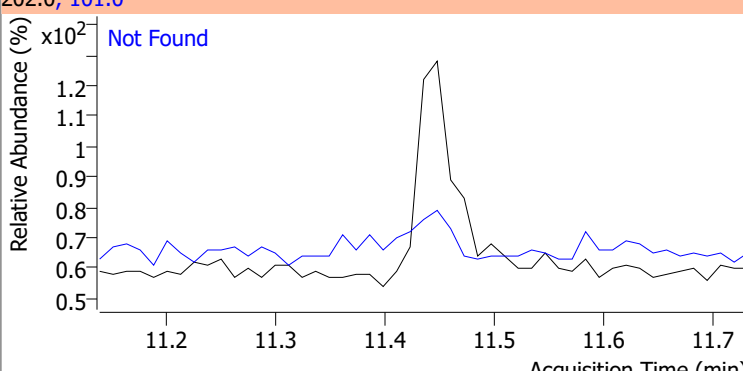
Compound	Conc.	Exp RT	QIon	Exp Ratio		
Phenanthrene	N.D.	9.82	176.0	15.5		
+ Selected Ion (178.0) Jan1030.D			178.0, 176.0			
						
Anthracene	N.D.	9.88	176.0	16.6		
+ Selected Ion (178.0) Jan1030.D			178.0, 176.0			
						
o-Terphenyl	N.D.	10.32	229.0	66.8	QIon	Exp Ratio
					215.0	43.2
+ Selected Ion (230.0) Jan1030.D			230.0, 229.0, 215.0			
						
Fluoranthene	N.D.	11.44	101.0	11.4		
+ Selected Ion (202.0) Jan1030.D			202.0, 101.0			
						

Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.6	30.8




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1031.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/11/2022 3:13:47 AM
Sample Name	B22010141-001C	Instrument	GCMS
Vial	31	Multiplier	1.00
DA Method File	011022 bna SIM 1.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 2.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	296583	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	520693	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	303447	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.793	188.0	685576	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	538344	40.0000	ng/ml	-0.013
M Perylene-d12	18.524	264.0	401795	40.0000	ng/ml	0.000
System Monitoring Compounds						
S Nitrobenzene-d5	5.143	82.0	629019	43.8272	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 876.54%		*
S 2-Fluorobiphenyl	7.265	172.0	989887	65.5250	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1310.50%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.300	244.0	1102071	110.6341	ng/ml	0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 2212.68%		*
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.013	154.0	0	ng/ml	md	1
T Fluorene	0.000		0	N.D.		
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.751	228.0	0	ng/ml	md	1
T Chrysene	14.751	228.0	0	ng/ml	md	1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.524	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	43.8272	5.14	-0.02	629019	54.0	33.3	21.6	40.2
					128.0	35.0	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	65.5250	7.26	0.00	989887	171.0	40.1	26.4	49.0




Compound	Conc.	Exp RT	QIon	Exp Ratio
Acenaphthylene	N.D.	7.84	153.0	14.6











Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene		0		0	153.0		80.3	149.2
					152.0		38.4	71.4



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Fluorene	N.D.	8.69	165.0	96.4	167.0	11.3




Quantitation Results Report (QT Reviewed)

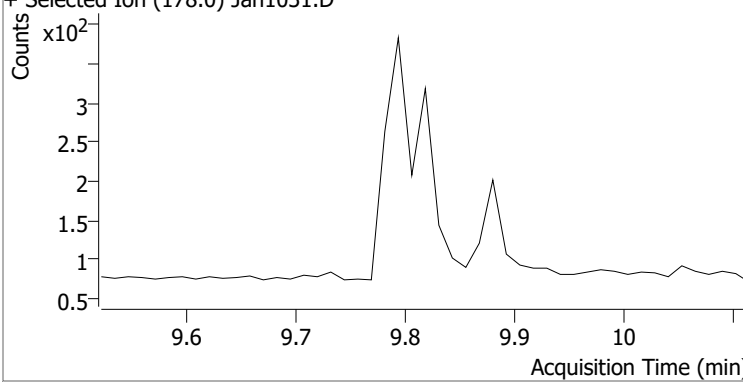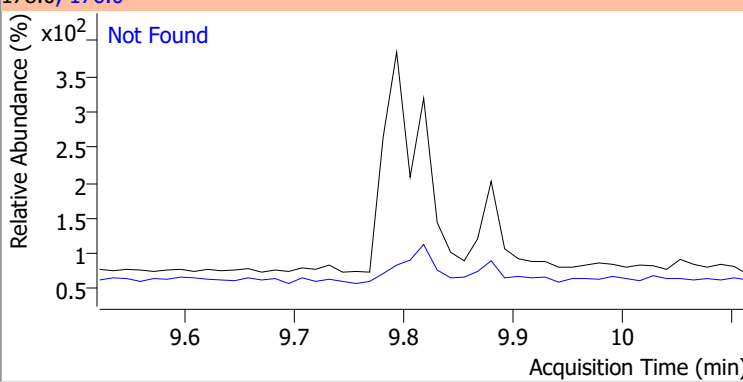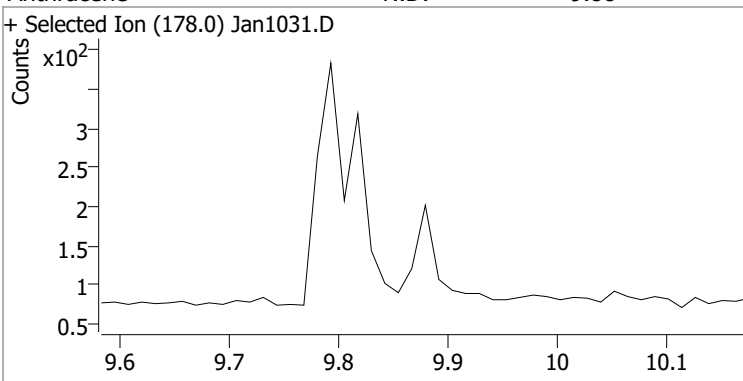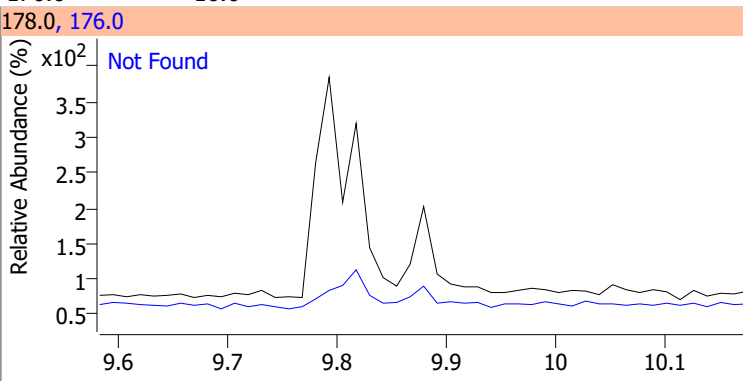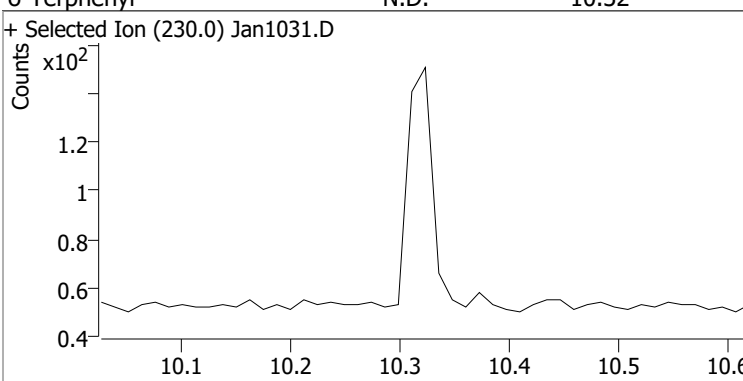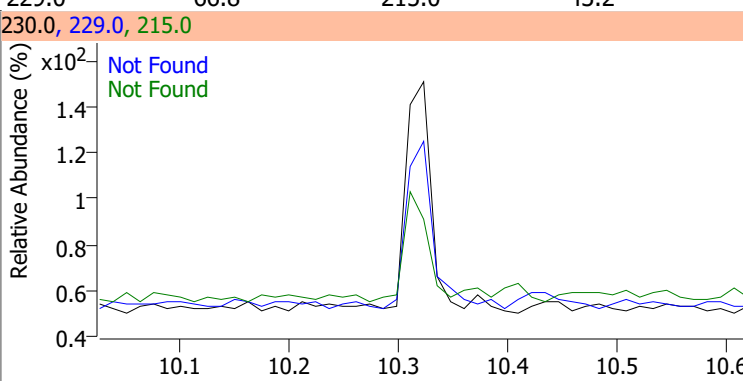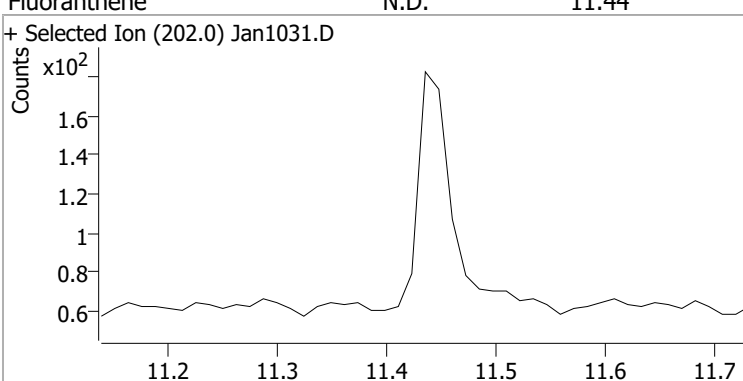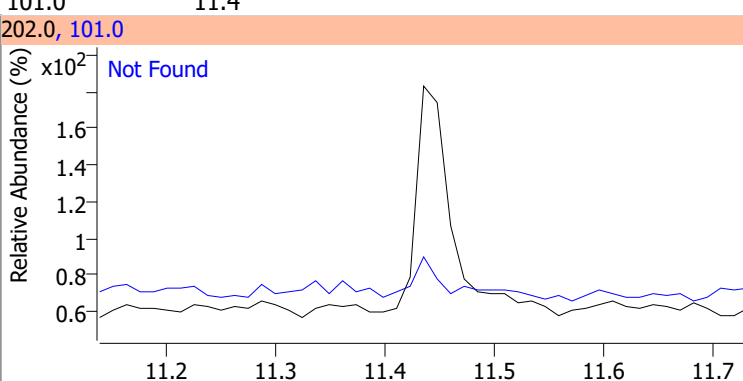
Compound	Conc.	Exp RT	QIon	Exp Ratio		
Phenanthrene	N.D.	9.82	176.0	15.5		
+ Selected Ion (178.0) Jan1031.D			178.0, 176.0			
						
Anthracene	N.D.	9.88	176.0	16.6		
+ Selected Ion (178.0) Jan1031.D			178.0, 176.0			
						
o-Terphenyl	N.D.	10.32	229.0	66.8	QIon	Exp Ratio
+ Selected Ion (230.0) Jan1031.D			230.0, 229.0, 215.0			
						
Fluoranthene	N.D.	11.44	101.0	11.4		
+ Selected Ion (202.0) Jan1031.D			202.0, 101.0			
						

Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Pyrene	N.D.	11.82	101.0	13.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	110.6341	12.30	0.01	1102071	122.0	14.5	9.6	17.9



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)Anthracene	0	0	0	0	226.0 229.0		19.5 16.5	36.3 30.6




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	0	0	0	0	226.0 229.0		22.2 15.5	41.2 28.9




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.6	30.8




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1032.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/11/2022 3:46:03 AM
Sample Name	B22010141-001C	Instrument	GCMS
Vial	32	Multiplier	20.00
DA Method File	011022 bna SIM 1.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 2.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	227113	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	447805	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	263315	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.793	188.0	588049	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	464039	40.0000	ng/ml	-0.013
M Perylene-d12	18.524	264.0	345842	40.0000	ng/ml	0.000
System Monitoring Compounds						
S Nitrobenzene-d5	5.156	82.0	16851	61.9545	ng/ml	-0.013
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 1239.09% *		
S 2-Fluorobiphenyl	7.264	172.0	44806	68.3587	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1367.17% *		
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.275	244.0	43434	101.1674	ng/ml	-0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 2023.35% *		
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.050	154.0	0		ng/ml md	1
T Fluorene	0.000		0	N.D.		
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.751	228.0	0		ng/ml md	1
T Chrysene	14.751	228.0	0		ng/ml md	1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.400	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	61.9545	5.16	-0.01	16851	54.0	30.9	21.6	40.2
					128.0	36.4	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4



Quantitation Results Report (QT Reviewed)

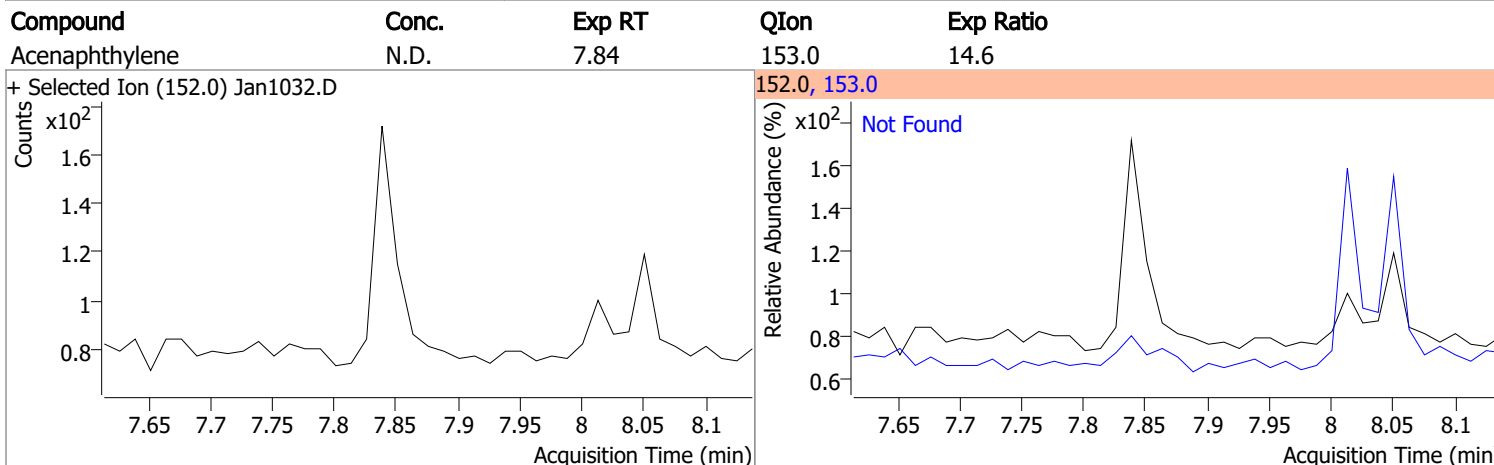


Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio		
Phenanthrene	N.D.	9.82	176.0	15.5		
+ Selected Ion (178.0) Jan1032.D			178.0, 176.0			
Anthracene	N.D.	9.88	176.0	16.6		
+ Selected Ion (178.0) Jan1032.D			178.0, 176.0			
o-Terphenyl	N.D.	10.32	229.0	66.8	QIon	Exp Ratio
+ Selected Ion (230.0) Jan1032.D			230.0, 229.0, 215.0			
Fluoranthene	N.D.	11.44	101.0	11.4		
+ Selected Ion (202.0) Jan1032.D			202.0, 101.0			

Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Pyrene	N.D.	11.82	101.0	13.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	101.1674	12.28	-0.01	43434	122.0	14.6	9.6	17.9



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)Anthracene	0	0	0	0	226.0		19.5	36.3
					229.0		16.5	30.6




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	0	0	0	0	226.0		22.2	41.2
					229.0		15.5	28.9




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.6	30.8




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1033.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/11/2022 4:18:30 AM
Sample Name	B22010141-001CLMS	Instrument	GCMS
Vial	33	Multiplier	1.00
DA Method File	011022 bna SIM 1.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 2.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	264908	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	445748	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	260140	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.793	188.0	600321	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	469314	40.0000	ng/ml	-0.013
M Perylene-d12	18.524	264.0	353152	40.0000	ng/ml	0.000
System Monitoring Compounds						
S Nitrobenzene-d5	5.156	82.0	19649	3.0968	ng/ml	# -0.013
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 61.94%		
S 2-Fluorobiphenyl	7.264	172.0	54343	4.1960	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 83.92%		
S o-Terphenyl	10.324	230.0	47109	4.2797	ng/ml	0.000
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = 85.59%		
S Terphenyl-d14	12.275	244.0	47964	5.5232	ng/ml	-0.013
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 110.46%		*
Target Compounds						
T Naphthalene	5.966	128.0	54956	3.6716	ng/ml	100
T 2-Methylnaphthalene	6.790	141.0	33408	3.8702	ng/ml	95
T 1-Methylnaphthalene	6.902	141.0	31773	3.9807	ng/ml	95
T Acenaphthylene	7.838	152.0	61778	4.4406	ng/ml	100
T Acenaphthene	8.050	154.0	42401	4.1920	ng/ml	99
T Fluorene	8.673	166.0	55438	4.7896	ng/ml	97
T Phenanthrene	9.817	178.0	86876	4.7976	ng/ml	91
T Anthracene	9.879	178.0	77810	5.0986	ng/ml	95
T Fluoranthene	11.435	202.0	99073	4.8415	ng/ml	100
T Pyrene	11.806	202.0	108672	4.6418	ng/ml	97
T Benzo(a)Anthracene	14.726	228.0	71997	5.0818	ng/ml	99
T Chrysene	14.813	228.0	98858	5.0651	ng/ml	98
T Benzo(b)fluoranthene	17.746	252.0	68814	4.5194	ng/ml	99


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	17.807	252.0	73133	4.4915	ng/ml	100
T Benzo(a)pyrene	18.388	252.0	51471	4.5096	ng/ml	99
T Indeno(1,2,3-cd)pyrene	20.241	276.0	48923	4.6265	ng/ml	96
T Dibenzo(a,h)anthracene	20.316	278.0	57836	4.7079	ng/ml	98
T Benzo(g,h,i)perylene	20.575	276.0	77416	4.7940	ng/ml	99


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	3.0968	5.16	-0.01	19649	54.0	43.6	21.6	40.2
					128.0	36.0	21.3	39.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	3.6716	5.97	-0.01	54956	102.0	15.6	0.0	46.6
					129.0	10.9	7.6	14.1






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	3.8702	6.79	-0.01	33408	142.0	144.6	103.3	191.8
					115.0	60.9	36.8	68.3






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	3.9807	6.90	0.00	31773	142.0	115.4	77.9	144.7
					115.0	58.6	44.4	82.5






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	4.1960	7.26	0.00	54343	171.0	36.2	26.4	49.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthylene	4.4406	7.84	0.00	61778	153.0	14.5	10.2	18.9






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	4.1920	8.05	0.00	42401	153.0	114.4	80.3	149.2
					152.0	54.2	38.4	71.4






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene	4.7896	8.67	-0.01	55438	165.0	99.5	67.5	125.3
					167.0	13.2	7.9	14.6






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Phenanthrene	4.7976	9.82	0.00	86876	176.0	19.3	10.9	20.2



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Anthracene	5.0986	9.88	0.00	77810	176.0	18.7	11.6	21.6




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
o-Terphenyl	4.2797	10.32	0.00	47109	229.0	67.9	46.7	86.8
					215.0	43.2	30.2	56.2




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluoranthene	4.8415	11.44	0.00	99073	101.0	11.3	8.0	14.8




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Pyrene	4.6418	11.81	-0.01	108672	101.0	12.8	9.7	18.1



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	5.5232	12.28	-0.01	47964	122.0	14.0	9.6	17.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)Anthracene	5.0818	14.73	0.00	71997	226.0 229.0	27.7 23.0	19.5 16.5	36.3 30.6




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	5.0651	14.81	-0.01	98858	226.0 229.0	30.6 21.4	22.2 15.5	41.2 28.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(b)fluoranthene	4.5194	17.75	-0.01	68814	253.0	22.4	15.8	29.4



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(k)fluoranthene	4.4915	17.81	-0.01	73133	253.0	23.0	16.1	30.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene	4.5096	18.39	-0.01	51471	253.0	24.4	16.6	30.8




Quantitation Results Report (QT Reviewed)

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Indeno(1,2,3-cd)pyrene	4.6265	20.24	0.00	48923	138.0	23.2	17.6	32.7
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1033.D</p> </div> <div style="width: 30%;"> <p>276.0, 138.0</p> <p>Ratio = 23.2 (92.2 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.241-20.241 min, 1 scans) (**) Jan1033.D</p> <p>Lib Match Score=78.7</p> </div> </div>								
Dibenzo(a,h)anthracene	4.7079	20.32	0.00	57836	279.0	26.8	18.1	33.6
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (278.0) Jan1033.D</p> </div> <div style="width: 30%;"> <p>278.0, 279.0, 139.0</p> <p>Ratio = 26.8 (103.7 %)</p> <p>Ratio = 18.8 (103.0 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.316-20.316 min, 1 scans) (**) Jan1033.D</p> <p>Lib Match Score=77.5</p> </div> </div>								
Benzo(g,h,i)perylene	4.7940	20.57	0.00	77416	277.0	25.0	17.1	31.8
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1033.D</p> </div> <div style="width: 30%;"> <p>276.0, 138.0, 277.0</p> <p>Ratio = 20.5 (102.6 %)</p> <p>Ratio = 25.0 (102.2 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.575-20.575 min, 1 scans) (**) Jan1033.D</p> <p>Lib Match Score=78.9</p> </div> </div>								

Quantitation Results Report (QT Reviewed)

Data File	Jan1034.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/11/2022 4:50:50 AM
Sample Name	B22010142-001C	Instrument	GCMS
Vial	34	Multiplier	1.00
DA Method File	011022 bna SIM 1.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 2.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	251538	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	441786	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	270434	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.793	188.0	569741	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	448261	40.0000	ng/ml	-0.013
M Perylene-d12	18.512	264.0	333287	40.0000	ng/ml	-0.012
System Monitoring Compounds						
S Nitrobenzene-d5	5.143	82.0	507750	42.4395	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 848.79%		*
S 2-Fluorobiphenyl	7.265	172.0	930574	69.1184	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1382.37%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.288	244.0	924393	111.4461	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 2228.92%		*
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.013	154.0	0		ng/ml	md
T Fluorene	0.000		0	N.D.		
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.751	228.0	0		ng/ml	md
T Chrysene	14.751	228.0	0		ng/ml	md
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.512	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	42.4395	5.14	-0.02	507750	54.0	33.2	21.6	40.2
					128.0	34.7	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4





Quantitation Results Report (QT Reviewed)

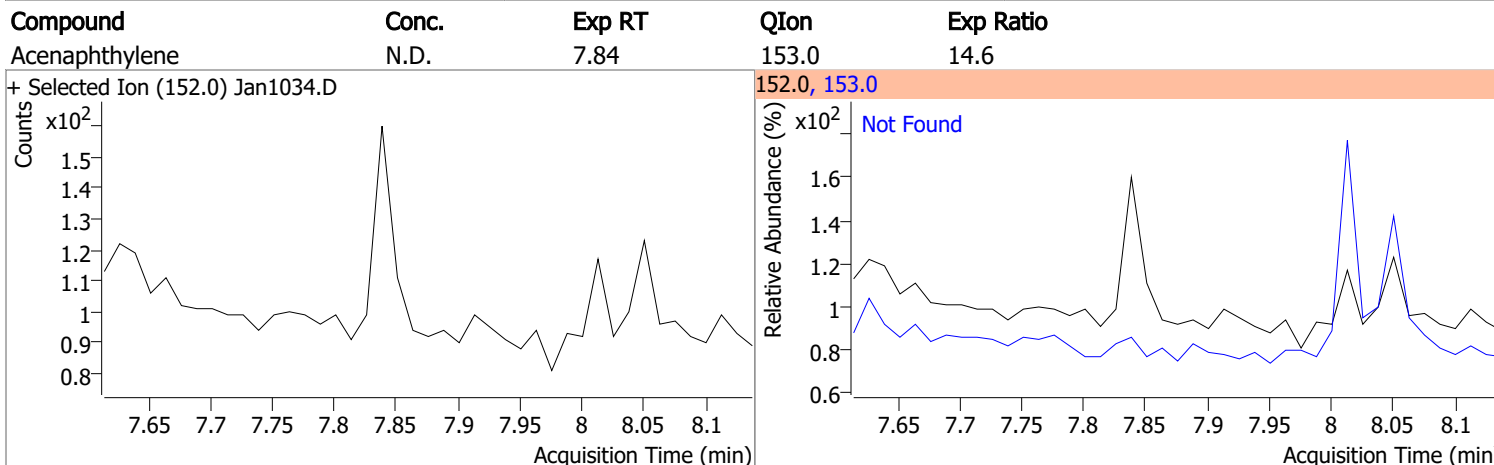



Quantitation Results Report (QT Reviewed)



Compound	Conc.	Exp RT	QIon	Exp Ratio
Phenanthrene	N.D.	9.82	176.0	15.5





Compound	Conc.	Exp RT	QIon	Exp Ratio
Anthracene	N.D.	9.88	176.0	16.6







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
o-Terphenyl	N.D.	10.32	229.0	66.8	215.0	43.2

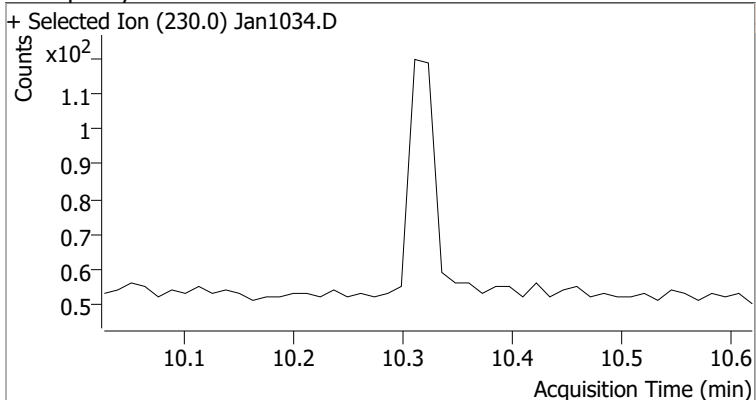

Compound	Conc.	Exp RT	QIon	Exp Ratio
Fluoranthene	N.D.	11.44	101.0	11.4




Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.6	30.8




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1035.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/11/2022 5:23:13 AM
Sample Name	B22010142-001C	Instrument	GCMS
Vial	35	Multiplier	20.00
DA Method File	011022 bna SIM 1.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 2.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	254106	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	441037	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	266439	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.793	188.0	574486	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	448868	40.0000	ng/ml	-0.013
M Perylene-d12	18.512	264.0	327940	40.0000	ng/ml	-0.012
System Monitoring Compounds						
S Nitrobenzene-d5	5.156	82.0	17240	57.0314	ng/ml	-0.013
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 1140.63%		*
S 2-Fluorobiphenyl	7.265	172.0	47617	71.7955	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1435.91%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.288	244.0	42796	103.0510	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 2061.02%		*
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.050	154.0	0		ng/ml md	1
T Fluorene	0.000		0	N.D.		
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.751	228.0	0		ng/ml md	1
T Chrysene	14.814	228.0	0		ng/ml md	1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.413	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	57.0314	5.16	-0.01	17240	54.0	29.6	21.6	40.2
					128.0	35.1	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	71.7955	7.26	0.00	47617	171.0	36.7	26.4	49.0




Compound	Conc.	Exp RT	QIon	Exp Ratio
Acenaphthylene	N.D.	7.84	153.0	14.6











Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene		0		0	153.0		80.3	149.2
					152.0		38.4	71.4







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Fluorene	N.D.	8.69	165.0	96.4	167.0	11.3



Quantitation Results Report (QT Reviewed)

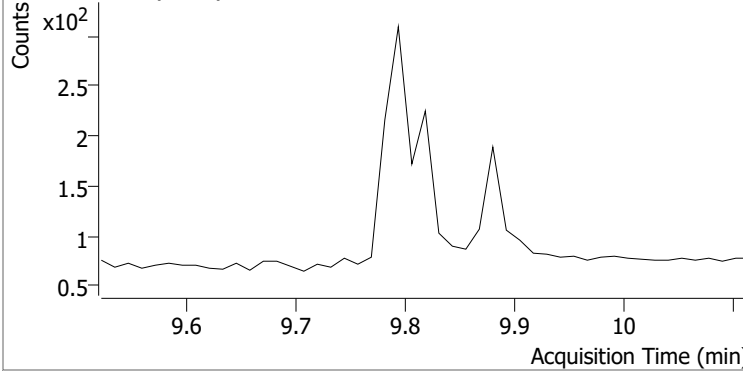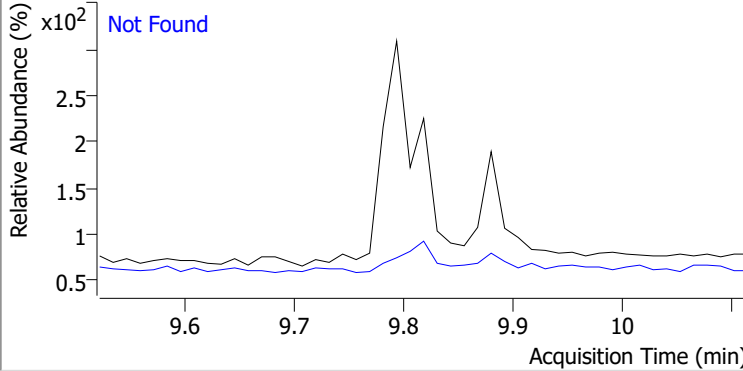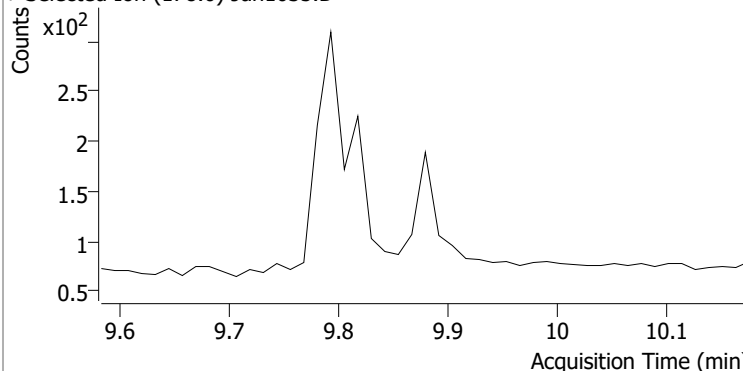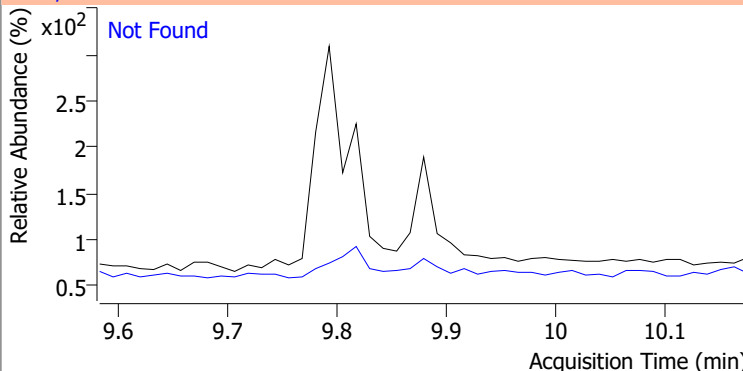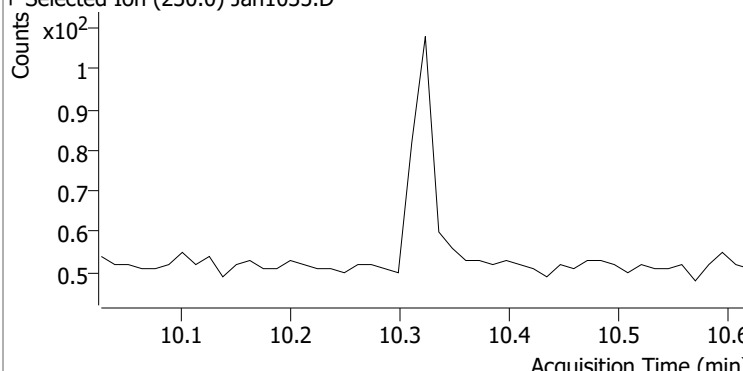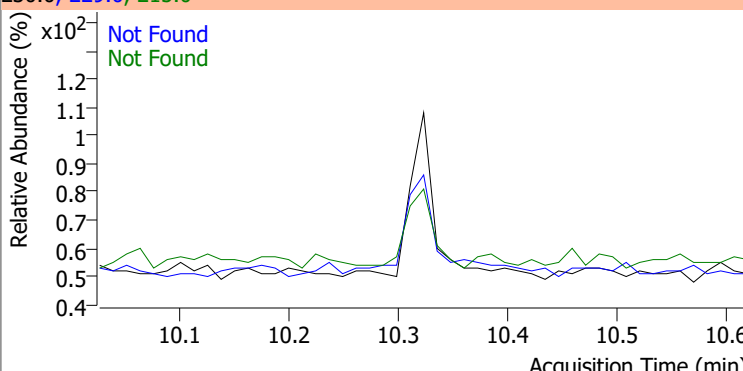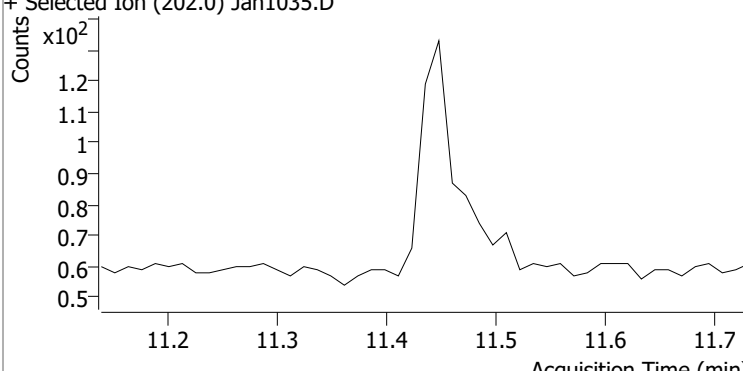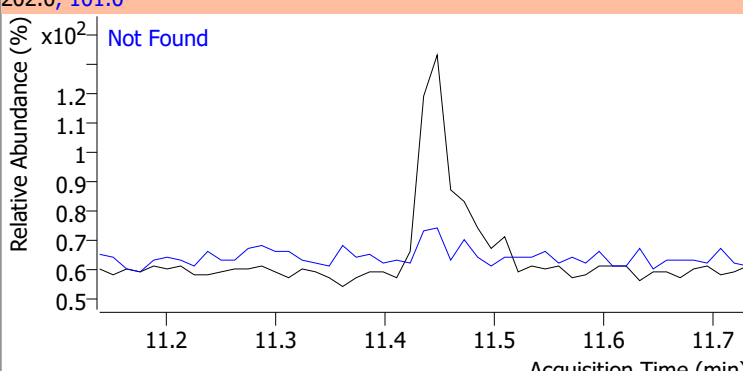
Compound	Conc.	Exp RT	QIon	Exp Ratio		
Phenanthrene	N.D.	9.82	176.0	15.5		
+ Selected Ion (178.0) Jan1035.D			178.0, 176.0			
						
Anthracene	N.D.	9.88	176.0	16.6		
+ Selected Ion (178.0) Jan1035.D			178.0, 176.0			
						
o-Terphenyl	N.D.	10.32	229.0	66.8	QIon	Exp Ratio
+ Selected Ion (230.0) Jan1035.D			230.0, 229.0, 215.0			
						
Fluoranthene	N.D.	11.44	101.0	11.4		
+ Selected Ion (202.0) Jan1035.D			202.0, 101.0			
						

Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.6	30.8




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1036.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/11/2022 5:55:27 AM
Sample Name	B22010143-001C	Instrument	GCMS
Vial	36	Multiplier	1.00
DA Method File	011022 bna SIM 1.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 2.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	282010	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	485762	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	294477	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.793	188.0	634867	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	502403	40.0000	ng/ml	-0.012
M Perylene-d12	18.512	264.0	370398	40.0000	ng/ml	-0.012
System Monitoring Compounds						
S Nitrobenzene-d5	5.143	82.0	536037	40.8014	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 816.03%		*
S 2-Fluorobiphenyl	7.265	172.0	1003387	68.4418	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1368.84%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.288	244.0	1014980	109.1804	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 2183.61%		*
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.050	154.0	0		ng/ml	md 1
T Fluorene	0.000		0	N.D.		
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.751	228.0	0		ng/ml	md 1
T Chrysene	14.814	228.0	0		ng/ml	md 1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.401	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	40.8014	5.14	-0.02	536037	54.0	34.3	21.6	40.2
					128.0	35.4	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4







Quantitation Results Report (QT Reviewed)

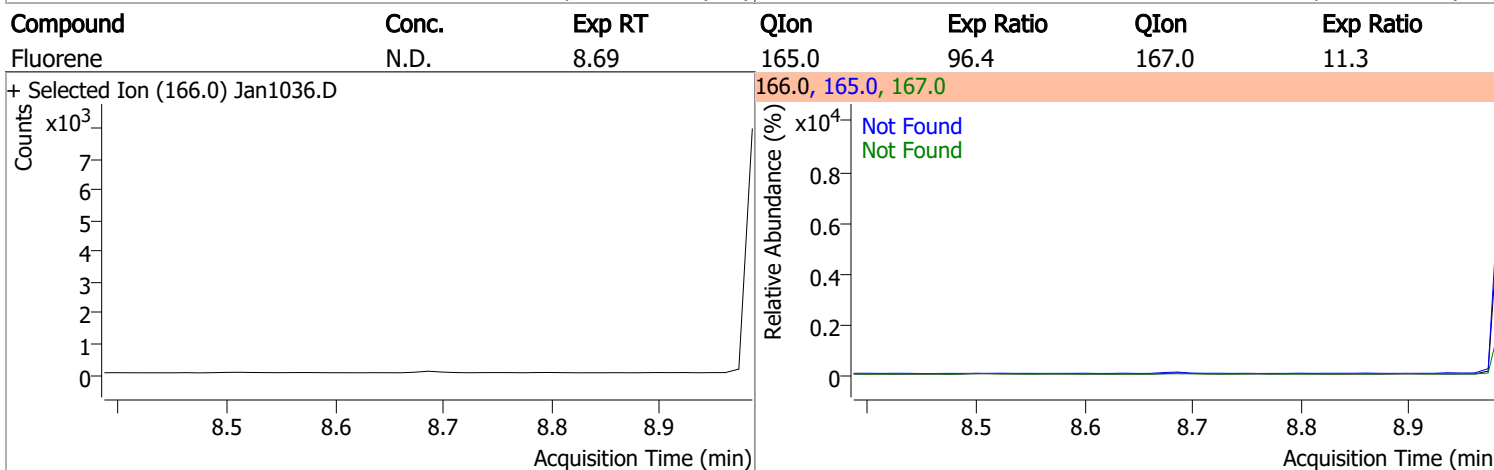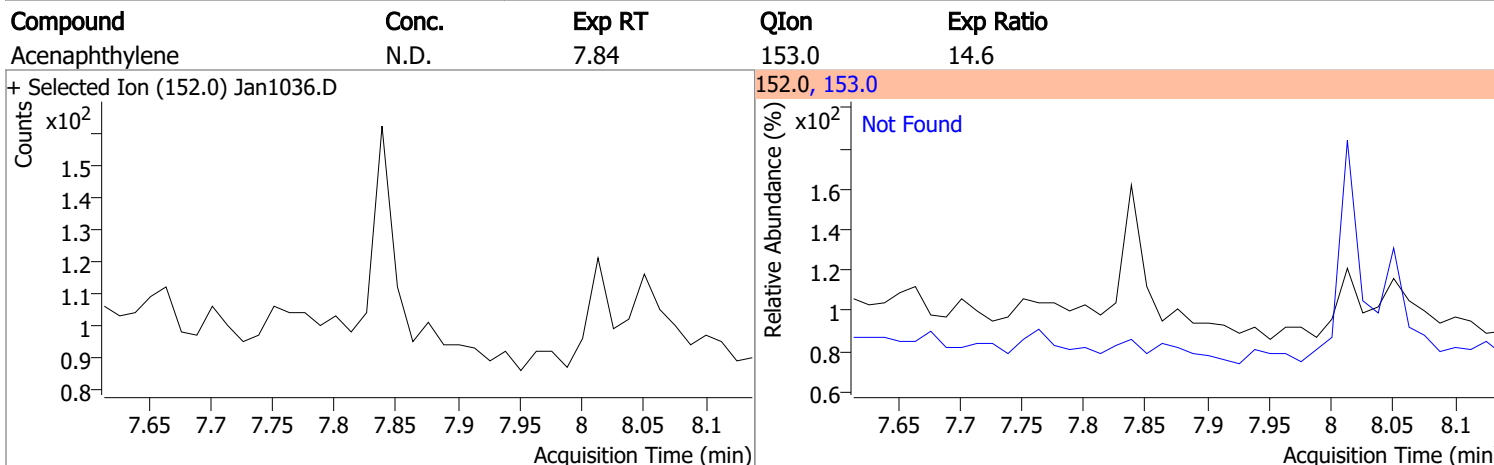

Quantitation Results Report (QT Reviewed)

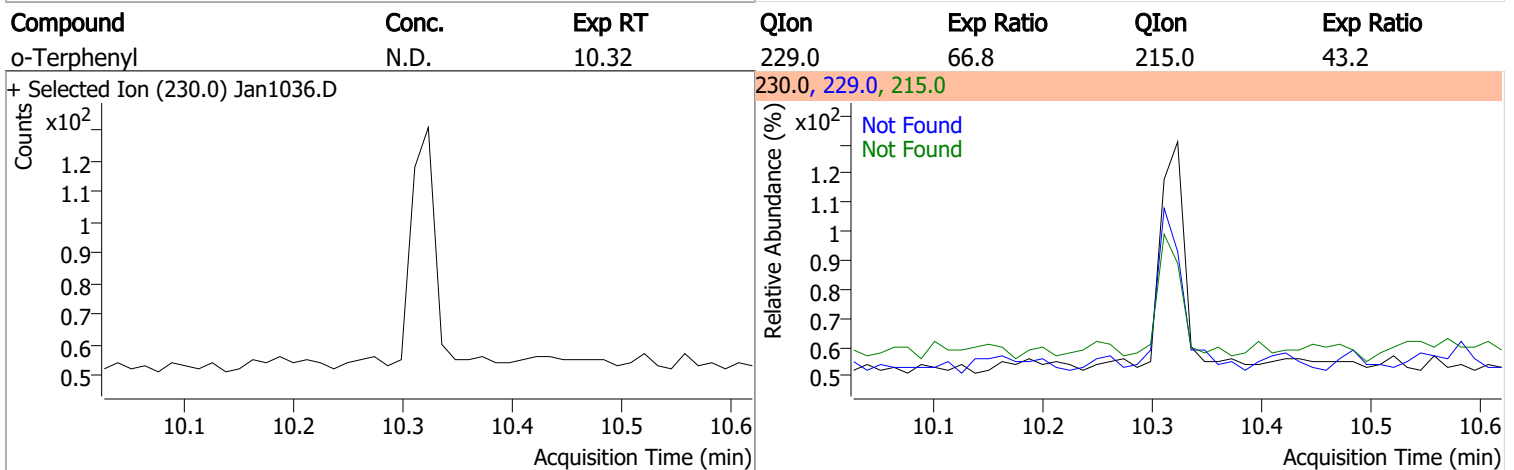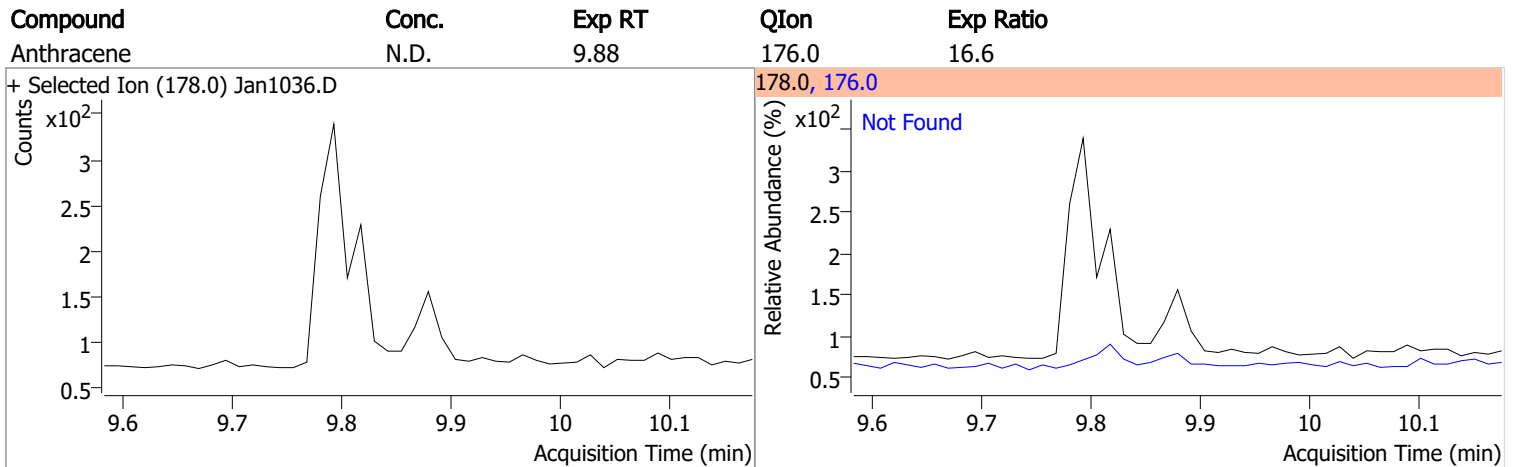


Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.6	30.8





Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2





Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1037.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/11/2022 6:27:51 AM
Sample Name	B22010143-001C	Instrument	GCMS
Vial	37	Multiplier	20.00
DA Method File	011022 bna SIM 1.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 2.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	274485	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	469321	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	281713	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.793	188.0	609232	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	474188	40.0000	ng/ml	-0.013
M Perylene-d12	18.512	264.0	356348	40.0000	ng/ml	-0.012
System Monitoring Compounds						
S Nitrobenzene-d5	5.156	82.0	18578	56.9042	ng/ml	-0.013
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 1138.08% *		
S 2-Fluorobiphenyl	7.264	172.0	49690	70.8596	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1417.19% *		
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.275	244.0	45561	103.8502	ng/ml	-0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 2077.00% *		
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.050	154.0	0		ng/ml md	1
T Fluorene	0.000		0	N.D.		
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.751	228.0	0		ng/ml md	1
T Chrysene	14.814	228.0	0		ng/ml md	1
T Benzo(b)fluoranthene	0.000		0	N.D.		




Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.400	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		



(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	56.9042	5.16	-0.01	18578	54.0	34.2	21.6	40.2
					128.0	36.5	21.3	39.5





Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4



Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Pyrene	N.D.	11.82	101.0	13.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	103.8502	12.28	-0.01	45561	122.0	14.0	9.6	17.9



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)Anthracene	0	0	0	0	226.0		19.5	36.3
					229.0		16.5	30.6




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	0	0	0	0	226.0		22.2	41.2
					229.0		15.5	28.9




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.6	30.8




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1038.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/11/2022 7:00:08 AM
Sample Name	B22010145-001C	Instrument	GCMS
Vial	38	Multiplier	1.00
DA Method File	011022 bna SIM 1.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 2.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	268395	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	473808	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	276513	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.793	188.0	606959	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	482068	40.0000	ng/ml	-0.013
M Perylene-d12	18.512	264.0	358353	40.0000	ng/ml	-0.013
System Monitoring Compounds						
S Nitrobenzene-d5	5.143	82.0	529954	41.8321	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 836.64%		*
S 2-Fluorobiphenyl	7.264	172.0	983114	71.4154	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1428.31%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.288	244.0	986455	110.5881	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 2211.76%		*
Target Compounds						QValue
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.050	154.0	0		ng/ml	md
T Fluorene	0.000		0	N.D.		
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.751	228.0	0		ng/ml	md
T Chrysene	14.813	228.0	0		ng/ml	md
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.512	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	41.8321	5.14	-0.03	529954	54.0	35.0	21.6	40.2
					128.0	33.8	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	71.4154	7.26	0.00	983114	171.0	39.8	26.4	49.0




Compound	Conc.	Exp RT	QIon	Exp Ratio
Acenaphthylene	N.D.	7.84	153.0	14.6



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene		0		0	153.0		80.3	149.2
					152.0		38.4	71.4




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Fluorene	N.D.	8.69	165.0	96.4	167.0	11.3




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Phenanthrene	N.D.	9.82	176.0	15.5




Compound	Conc.	Exp RT	QIon	Exp Ratio
Anthracene	N.D.	9.88	176.0	16.6



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
o-Terphenyl	N.D.	10.32	229.0	66.8	215.0	43.2




Compound	Conc.	Exp RT	QIon	Exp Ratio
Fluoranthene	N.D.	11.44	101.0	11.4




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Pyrene	N.D.	11.82	101.0	13.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	110.5881	12.29	0.00	986455	122.0	14.6	9.6	17.9











Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)Anthracene		0		0	226.0		19.5	36.3
					229.0		16.5	30.6



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene		0		0	226.0		22.2	41.2
					229.0		15.5	28.9




Quantitation Results Report (QT Reviewed)

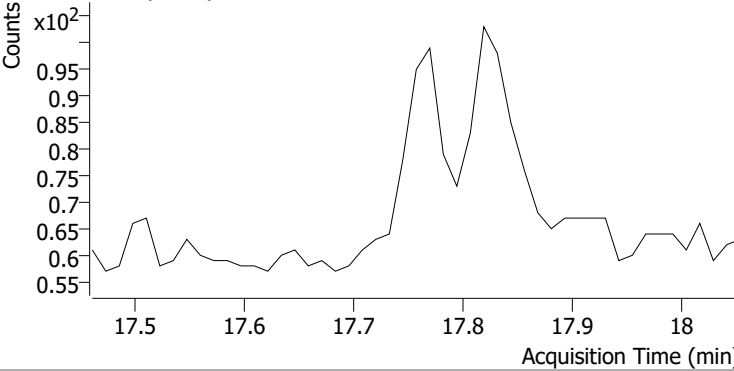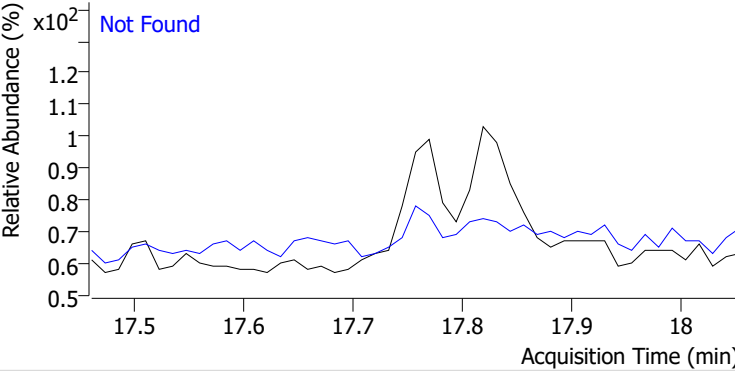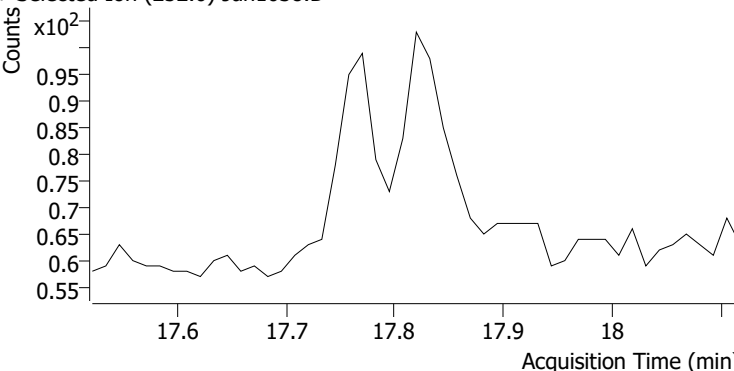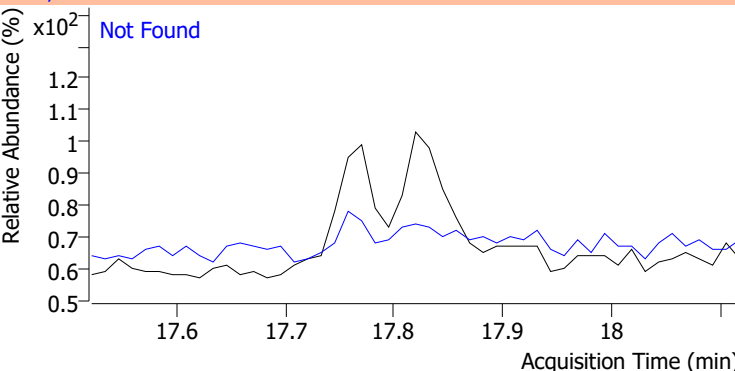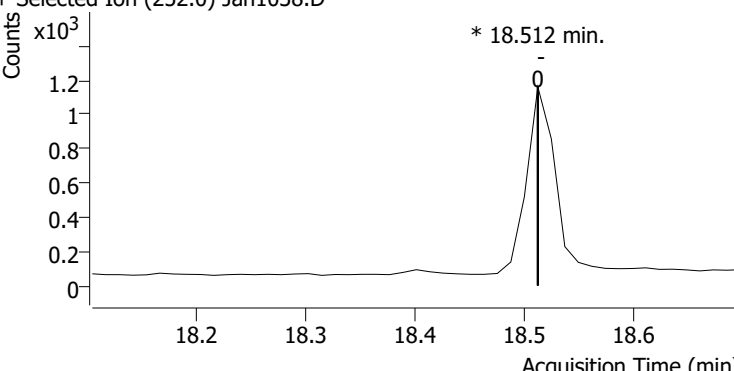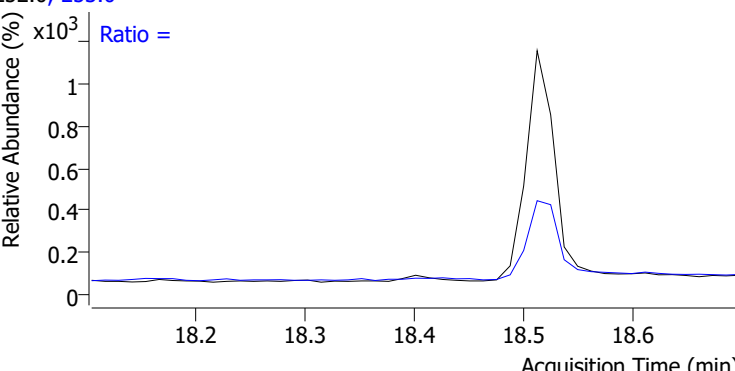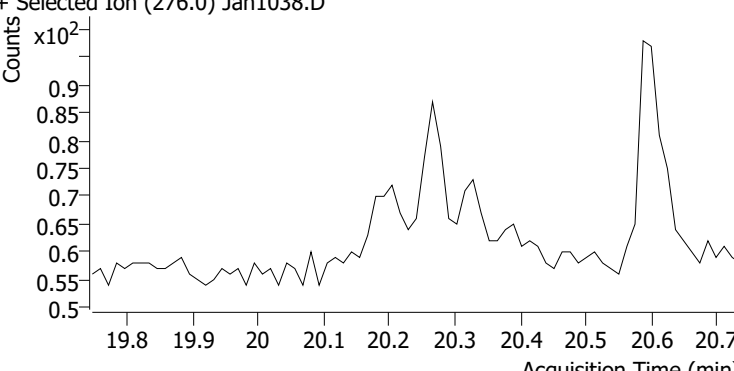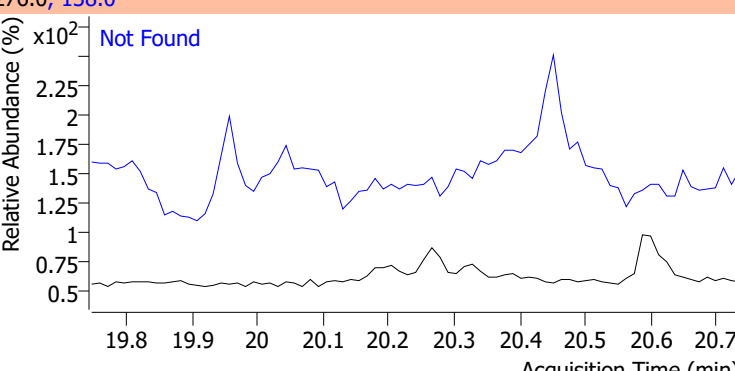
Compound	Conc.	Exp RT	QIon	Exp Ratio				
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6				
+ Selected Ion (252.0) Jan1038.D		252.0, 253.0						
								
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0				
+ Selected Ion (252.0) Jan1038.D		252.0, 253.0						
								
Benzo(a)pyrene		RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
		0		0	253.0		16.6	30.8
+ Selected Ion (252.0) Jan1038.D		252.0, 253.0						
								
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2				
+ Selected Ion (276.0) Jan1038.D		276.0, 138.0						
								

Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1039.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/11/2022 7:32:26 AM
Sample Name	B22010145-001C	Instrument	GCMS
Vial	39	Multiplier	20.00
DA Method File	011022 bna SIM 1.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 2.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	239188	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	456379	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	274582	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.793	188.0	589075	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	466798	40.0000	ng/ml	-0.013
M Perylene-d12	18.512	264.0	343661	40.0000	ng/ml	-0.012
System Monitoring Compounds						
S Nitrobenzene-d5	5.156	82.0	17919	62.5060	ng/ml	-0.013
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 1250.12%		*
S 2-Fluorobiphenyl	7.264	172.0	49898	73.0039	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1460.08%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.275	244.0	47386	109.7218	ng/ml	-0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 2194.44%		*
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.050	154.0	0		ng/ml	md
T Fluorene	0.000		0	N.D.		
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.751	228.0	0		ng/ml	md
T Chrysene	14.814	228.0	0		ng/ml	md
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.400	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	62.5060	5.16	-0.01	17919	54.0	31.3	21.6	40.2
					128.0	35.4	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	73.0039	7.26	0.00	49898	171.0	36.6	26.4	49.0




Compound	Conc.	Exp RT	QIon	Exp Ratio
Acenaphthylene	N.D.	7.84	153.0	14.6



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene		0		0	153.0 152.0		80.3 38.4	149.2 71.4







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Fluorene	N.D.	8.69	165.0	96.4	167.0	11.3



Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio		
Phenanthrene	N.D.	9.82	176.0	15.5		
+ Selected Ion (178.0) Jan1039.D			178.0, 176.0			
Anthracene	N.D.	9.88	176.0	16.6		
+ Selected Ion (178.0) Jan1039.D			178.0, 176.0			
o-Terphenyl	N.D.	10.32	229.0	66.8	QIon	Exp Ratio
+ Selected Ion (230.0) Jan1039.D			230.0, 229.0, 215.0			
Fluoranthene	N.D.	11.44	101.0	11.4		
+ Selected Ion (202.0) Jan1039.D			202.0, 101.0			

Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.6	30.8




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1040.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/11/2022 8:04:43 AM
Sample Name	B22010148-001C	Instrument	GCMS
Vial	40	Multiplier	1.00
DA Method File	011022 bna SIM 1.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 2.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	277857	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	501103	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	304271	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.793	188.0	625008	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	492298	40.0000	ng/ml	-0.013
M Perylene-d12	18.512	264.0	366656	40.0000	ng/ml	-0.012
System Monitoring Compounds						
S Nitrobenzene-d5	5.143	82.0	510329	39.8907	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 797.81%		*
S 2-Fluorobiphenyl	7.265	172.0	950923	62.7754	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1255.51%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.288	244.0	975699	107.1093	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 2142.19%		*
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.050	154.0	0		ng/ml	md 1
T Fluorene	8.985	166.0	0		ng/ml	md 1
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.751	228.0	0		ng/ml	md 1
T Chrysene	14.814	228.0	0		ng/ml	md 1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.512	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	39.8907	5.14	-0.02	510329	54.0	34.9	21.6	40.2
					128.0	32.3	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	62.7754	7.26	0.00	950923	171.0	38.8	26.4	49.0




Compound	Conc.	Exp RT	QIon	Exp Ratio
Acenaphthylene	N.D.	7.84	153.0	14.6



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene		0		0	153.0		80.3	149.2
					152.0		38.4	71.4




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene		0		0	165.0		67.5	125.3
					167.0		7.9	14.6




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Phenanthrene	N.D.	9.82	176.0	15.5




Compound	Conc.	Exp RT	QIon	Exp Ratio
Anthracene	N.D.	9.88	176.0	16.6



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
o-Terphenyl	N.D.	10.32	229.0	66.8	215.0	43.2




Compound	Conc.	Exp RT	QIon	Exp Ratio
Fluoranthene	N.D.	11.44	101.0	11.4




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Pyrene	N.D.	11.82	101.0	13.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	107.1093	12.29	0.00	975699	122.0	14.9	9.6	17.9



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)Anthracene	0	0	0	0	226.0 229.0		19.5 16.5	36.3 30.6




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	0	0	0	0	226.0 229.0		22.2 15.5	41.2 28.9




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.6	30.8




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1041.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/11/2022 8:37:11 AM
Sample Name	B22010148-001C	Instrument	GCMS
Vial	41	Multiplier	20.00
DA Method File	011022 bna SIM 1.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 2.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	223693	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	420066	40.0000	ng/ml	-0.012
M Acenaphthene-d10	8.013	164.0	258853	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.793	188.0	528412	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	417249	40.0000	ng/ml	-0.012
M Perylene-d12	18.512	264.0	311686	40.0000	ng/ml	-0.012
System Monitoring Compounds						
S Nitrobenzene-d5	5.156	82.0	14514	54.7149	ng/ml	-0.012
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 1094.30%		*
S 2-Fluorobiphenyl	7.265	172.0	40723	63.1999	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1264.00%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.275	244.0	41295	106.9728	ng/ml	-0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 2139.46%		*
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.050	154.0	0		ng/ml	md
T Fluorene	0.000		0	N.D.		
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.739	228.0	0		ng/ml	md
T Chrysene	14.814	228.0	0		ng/ml	md
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.401	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	54.7149	5.16	-0.01	14514	54.0	31.7	21.6	40.2
					128.0	36.8	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5











Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4



Quantitation Results Report (QT Reviewed)

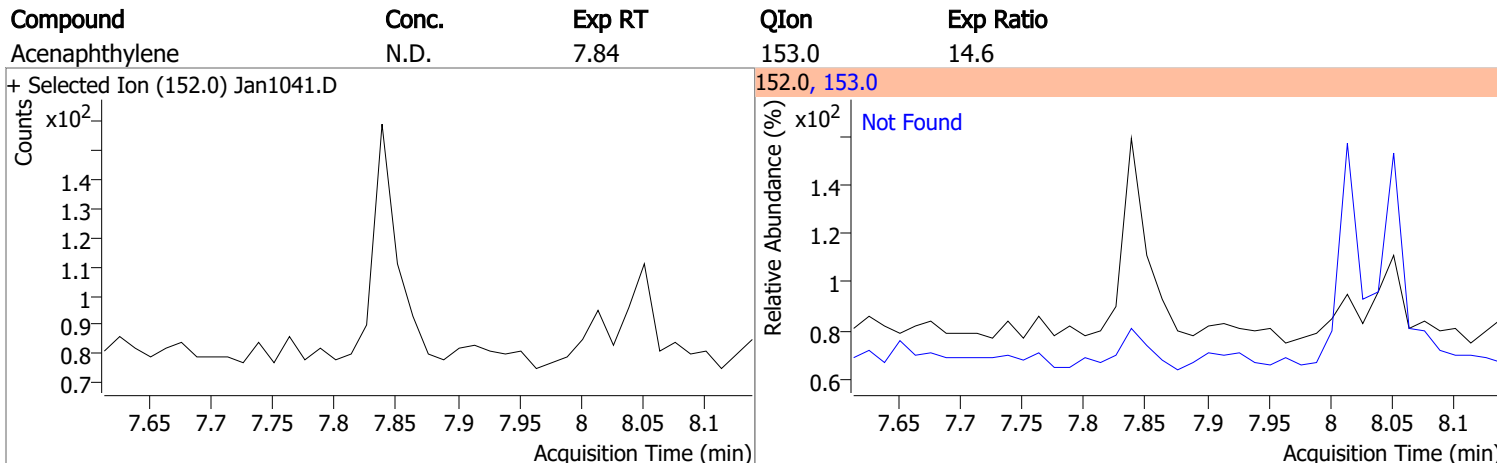


Quantitation Results Report (QT Reviewed)

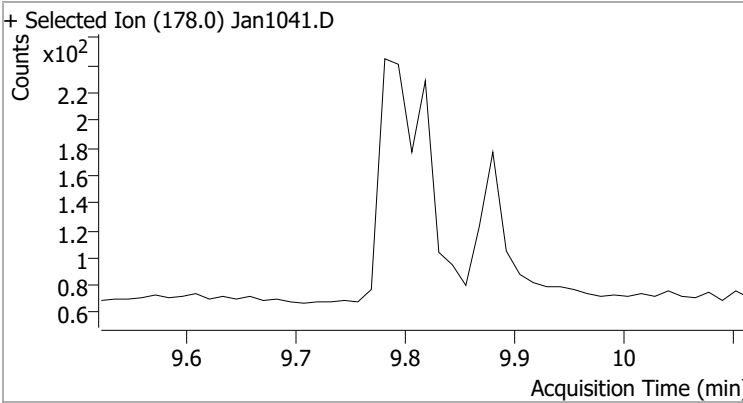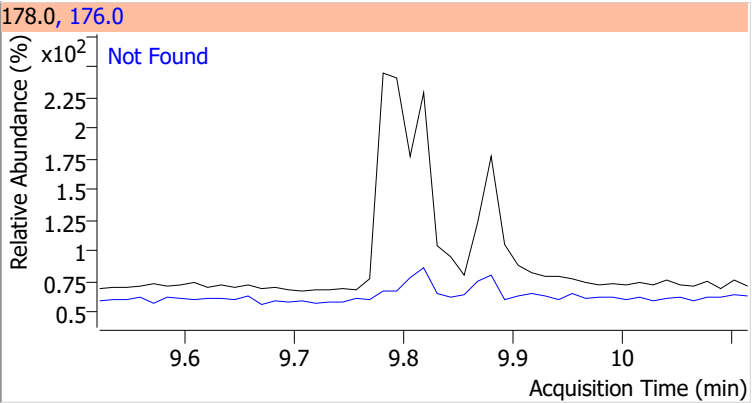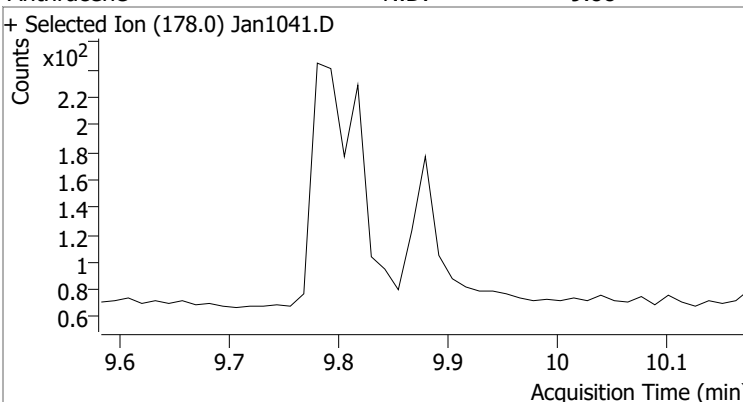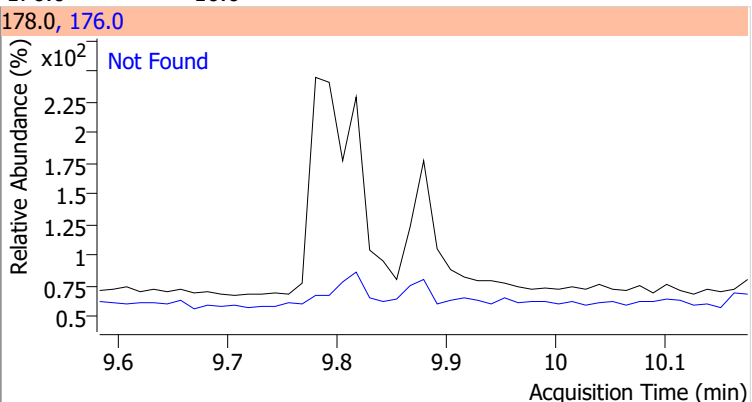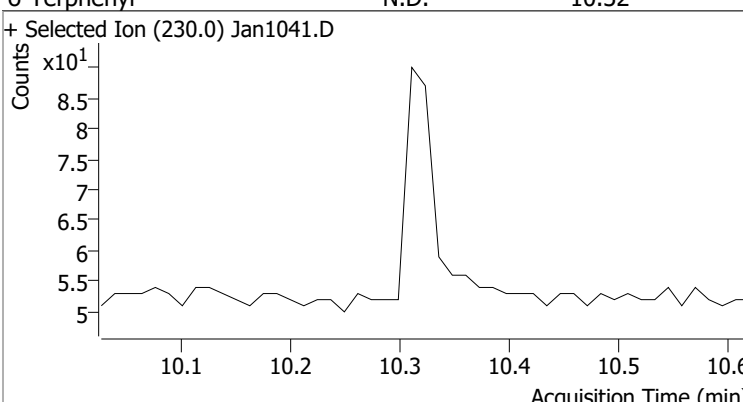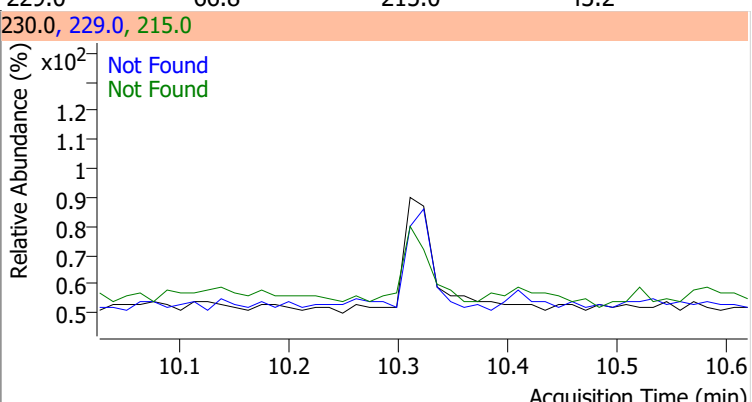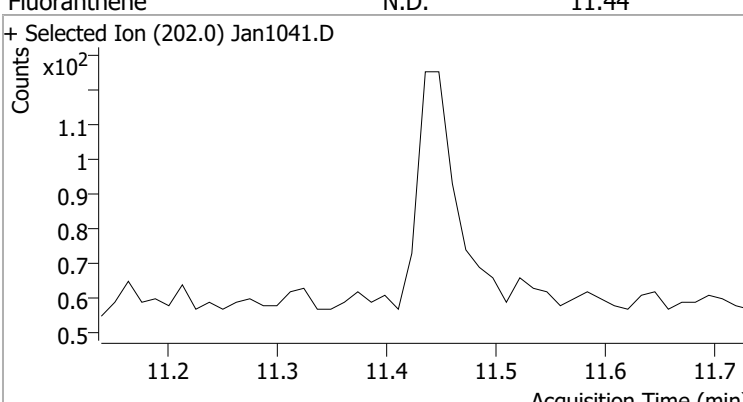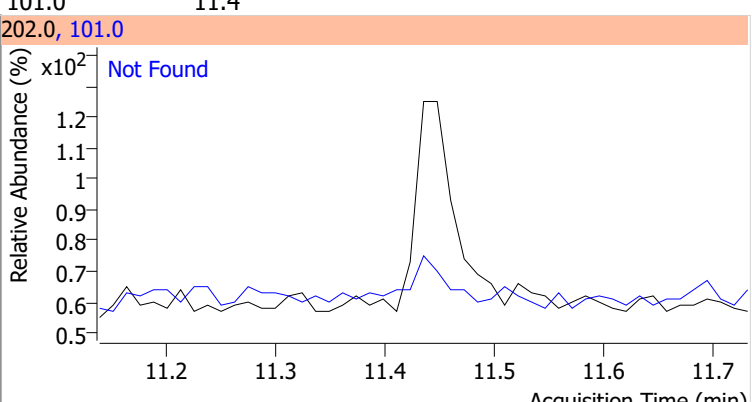
Compound	Conc.	Exp RT	QIon	Exp Ratio		
Phenanthrene	N.D.	9.82	176.0	15.5		
+ Selected Ion (178.0) Jan1041.D 			178.0, 176.0 			
Anthracene	N.D.	9.88	176.0	16.6		
+ Selected Ion (178.0) Jan1041.D 			178.0, 176.0 			
o-Terphenyl	N.D.	10.32	229.0	66.8	QIon	Exp Ratio
			215.0	43.2		
+ Selected Ion (230.0) Jan1041.D 			230.0, 229.0, 215.0 			
Fluoranthene	N.D.	11.44	101.0	11.4		
+ Selected Ion (202.0) Jan1041.D 			202.0, 101.0 			

Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Pyrene	N.D.	11.82	101.0	13.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	106.9728	12.28	-0.01	41295	122.0	14.0	9.6	17.9



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)Anthracene	0	0	0	0	226.0		19.5	36.3
					229.0		16.5	30.6




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	0	0	0	0	226.0		22.2	41.2
					229.0		15.5	28.9




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.6	30.8




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1042.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/11/2022 9:09:37 AM
Sample Name	B22010209-001C	Instrument	GCMS
Vial	42	Multiplier	1.00
DA Method File	011022 bna SIM 1.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 2.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	260961	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	461070	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	282539	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.780	188.0	587437	40.0000	ng/ml	-0.012
M Chrysene-d12	14.751	240.0	455522	40.0000	ng/ml	-0.013
M Perylene-d12	18.512	264.0	339689	40.0000	ng/ml	-0.012
System Monitoring Compounds						
S Nitrobenzene-d5	5.143	82.0	441042	37.7531	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 755.06%		*
S 2-Fluorobiphenyl	7.265	172.0	737405	52.4241	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1048.48%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.288	244.0	837827	99.3995	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 1987.99%		*
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.050	154.0	0		ng/ml	md 1
T Fluorene	8.686	166.0	0		ng/ml	md 1
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.751	228.0	0		ng/ml	md 1
T Chrysene	14.751	228.0	0		ng/ml	md 1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.413	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	37.7531	5.14	-0.02	441042	54.0	35.3	21.6	40.2
					128.0	32.1	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5











Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4







Quantitation Results Report (QT Reviewed)

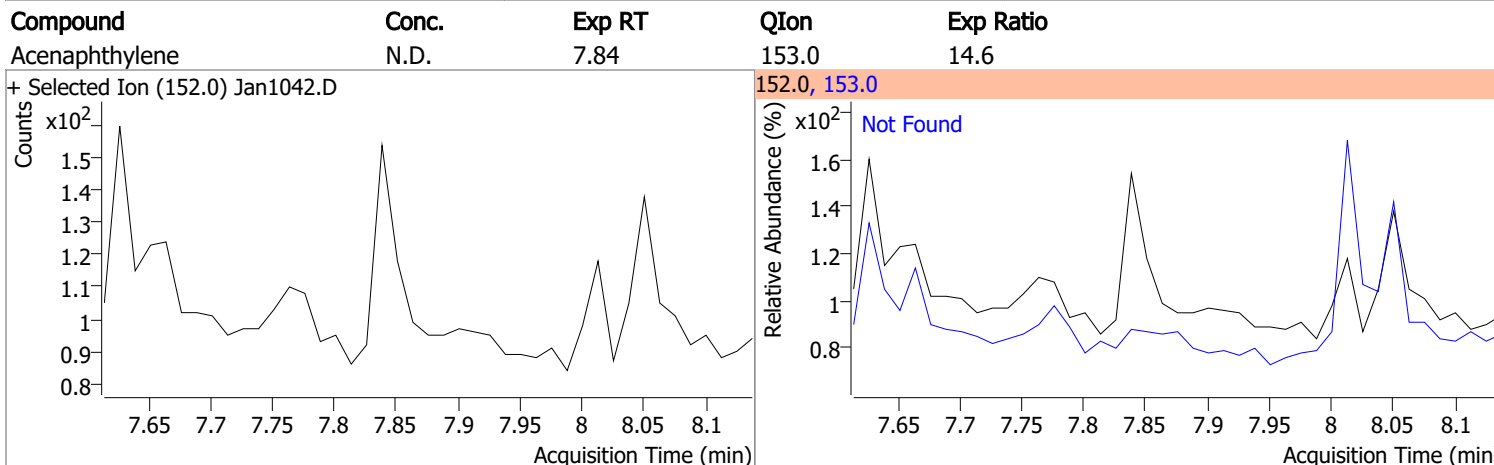

Quantitation Results Report (QT Reviewed)

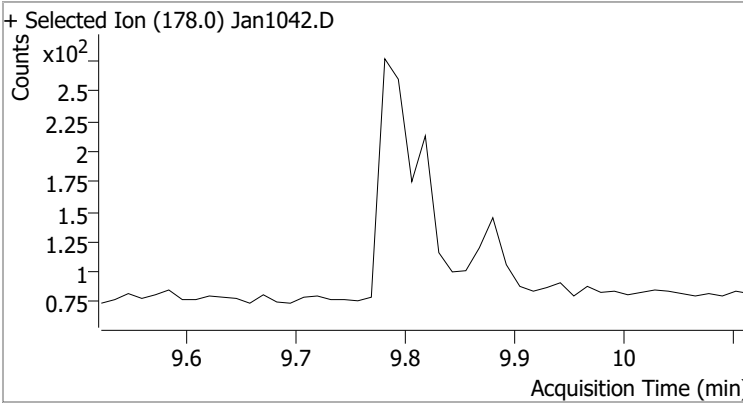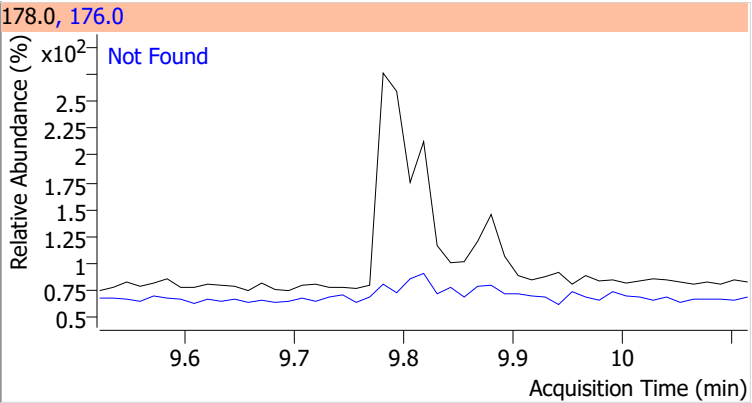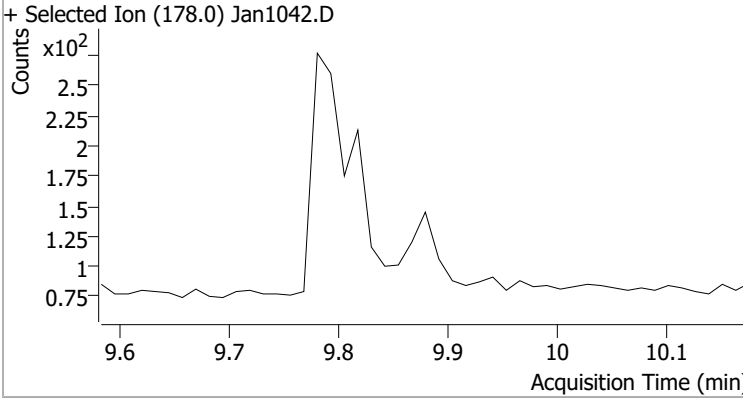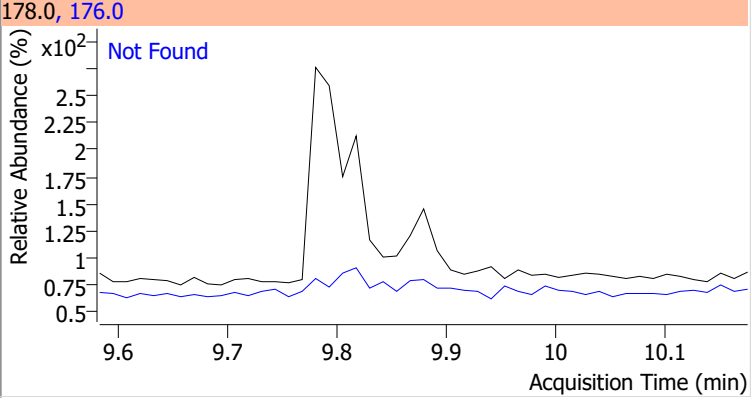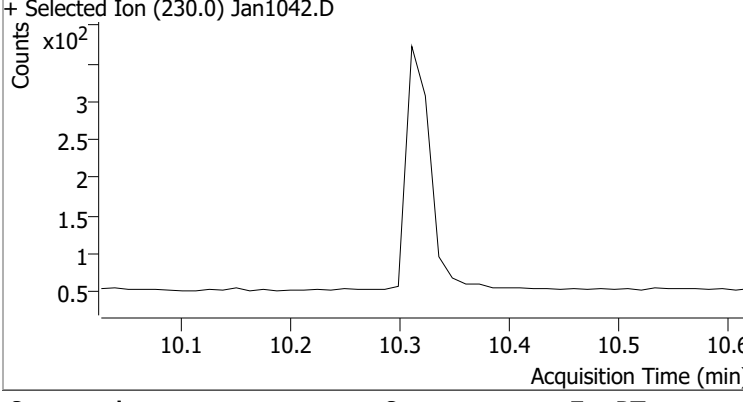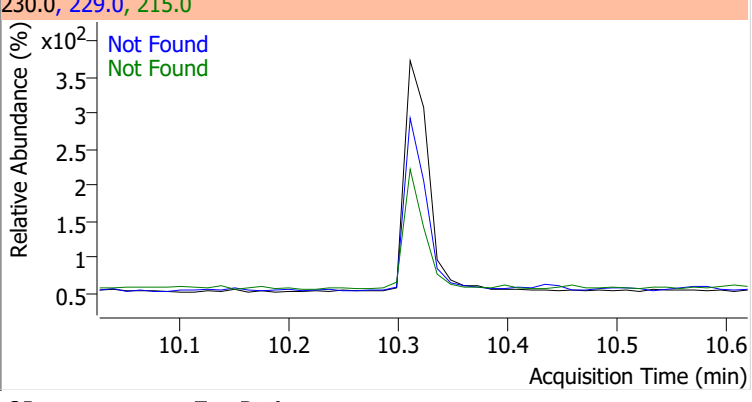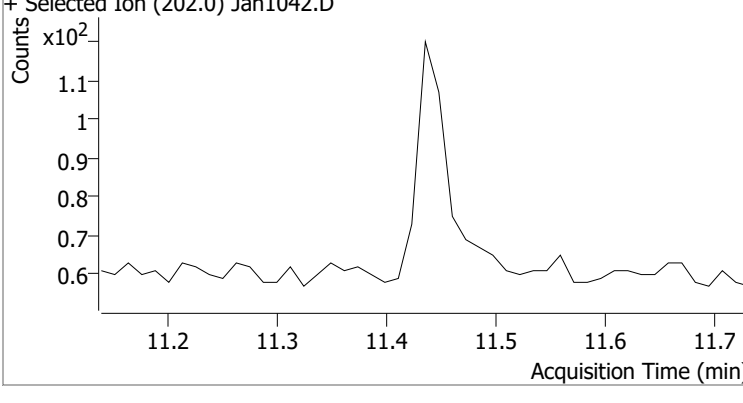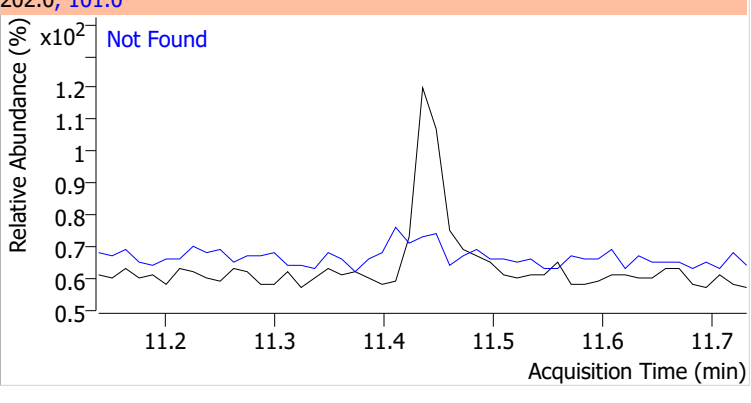
Compound	Conc.	Exp RT	QIon	Exp Ratio		
Phenanthrene	N.D.	9.82	176.0	15.5		
+ Selected Ion (178.0) Jan1042.D			178.0, 176.0			
						
Anthracene	N.D.	9.88	176.0	16.6		
+ Selected Ion (178.0) Jan1042.D			178.0, 176.0			
						
o-Terphenyl	N.D.	10.32	229.0	66.8	QIon	Exp Ratio
+ Selected Ion (230.0) Jan1042.D			230.0, 229.0, 215.0			
						
Fluoranthene	N.D.	11.44	101.0	11.4		
+ Selected Ion (202.0) Jan1042.D			202.0, 101.0			
						

Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.6	30.8




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1043.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/11/2022 9:42:03 AM
Sample Name	B22010209-001C	Instrument	GCMS
Vial	43	Multiplier	20.00
DA Method File	011022 bna SIM 1.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 2.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	276310	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	474264	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	285355	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.793	188.0	624859	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	492269	40.0000	ng/ml	-0.013
M Perylene-d12	18.512	264.0	369405	40.0000	ng/ml	-0.012
System Monitoring Compounds						
S Nitrobenzene-d5	5.156	82.0	15700	48.3475	ng/ml	-0.013
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 966.95%		*
S 2-Fluorobiphenyl	7.265	172.0	39264	55.2765	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1105.53%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.275	244.0	44301	97.2703	ng/ml	-0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 1945.41%		*
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.050	154.0	0		ng/ml md	1
T Fluorene	0.000		0	N.D.		
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.751	228.0	0		ng/ml md	1
T Chrysene	14.751	228.0	0		ng/ml md	1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.400	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	48.3475	5.16	-0.01	15700	54.0	31.1	21.6	40.2
					128.0	35.3	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5






Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4





Quantitation Results Report (QT Reviewed)



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	55.2765	7.26	0.00	39264	171.0	35.8	26.4	49.0





Compound	Conc.	Exp RT	QIon	Exp Ratio
Acenaphthylene	N.D.	7.84	153.0	14.6











Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene		0		0	153.0		80.3	149.2
					152.0		38.4	71.4



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Fluorene	N.D.	8.69	165.0	96.4	167.0	11.3




Quantitation Results Report (QT Reviewed)

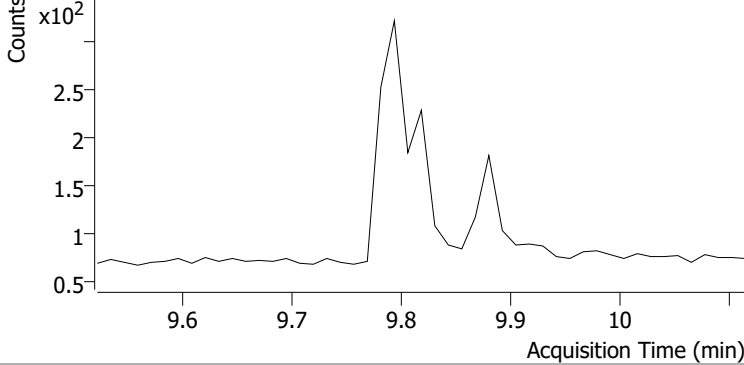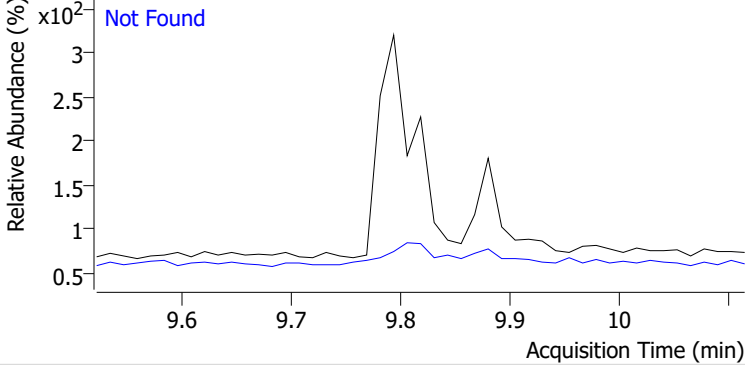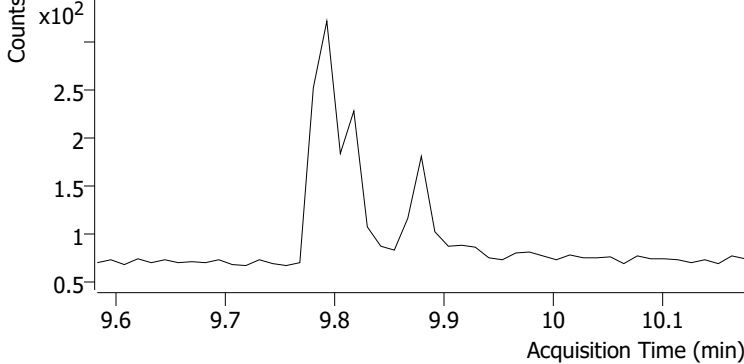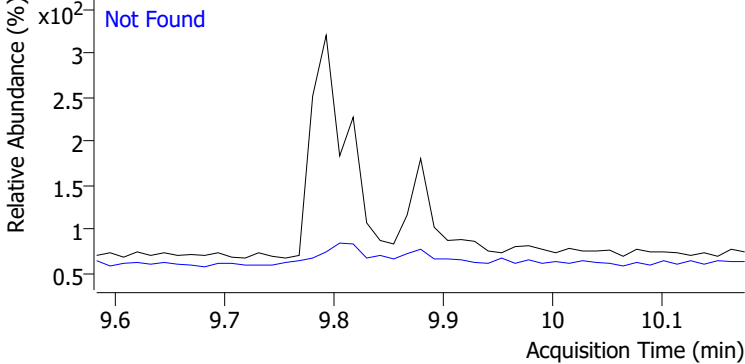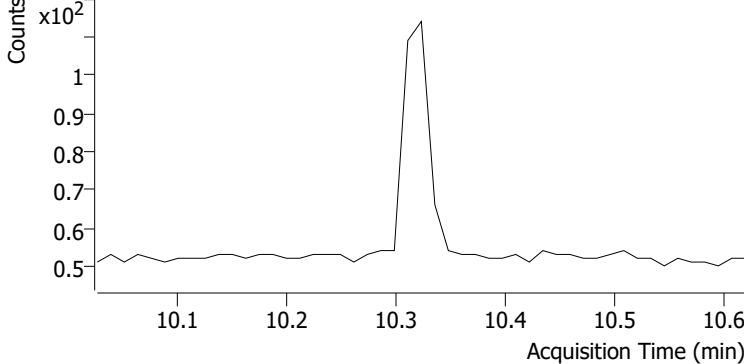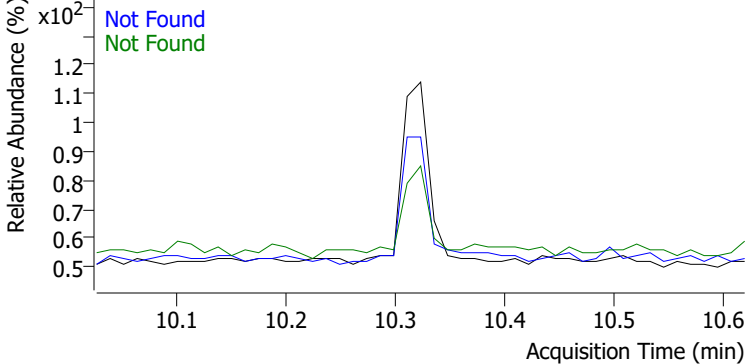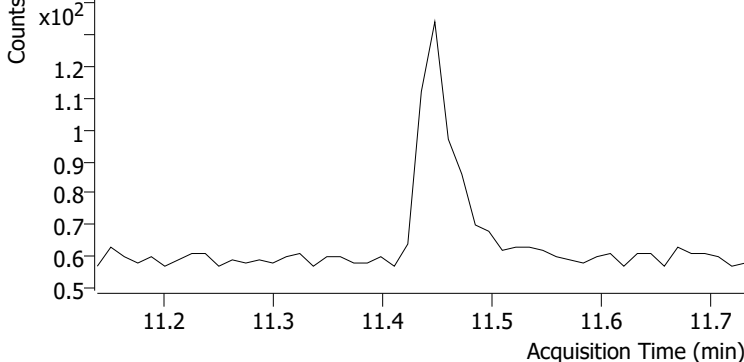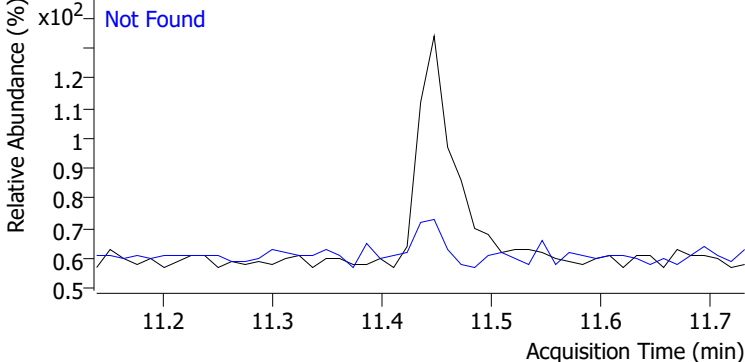
Compound	Conc.	Exp RT	QIon	Exp Ratio		
Phenanthrene	N.D.	9.82	176.0	15.5		
+ Selected Ion (178.0) Jan1043.D			178.0, 176.0			
						
Anthracene	N.D.	9.88	176.0	16.6		
+ Selected Ion (178.0) Jan1043.D			178.0, 176.0			
						
o-Terphenyl	N.D.	10.32	229.0	66.8	QIon	Exp Ratio
			215.0	43.2		
+ Selected Ion (230.0) Jan1043.D			230.0, 229.0, 215.0			
						
Fluoranthene	N.D.	11.44	101.0	11.4		
+ Selected Ion (202.0) Jan1043.D			202.0, 101.0			
						

Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Pyrene	N.D.	11.82	101.0	13.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	97.2703	12.28	-0.01	44301	122.0	14.6	9.6	17.9







Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)Anthracene	0	0	0	0	226.0 229.0		19.5 16.5	36.3 30.6



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	0	0	0	0	226.0 229.0		22.2 15.5	41.2 28.9




Quantitation Results Report (QT Reviewed)

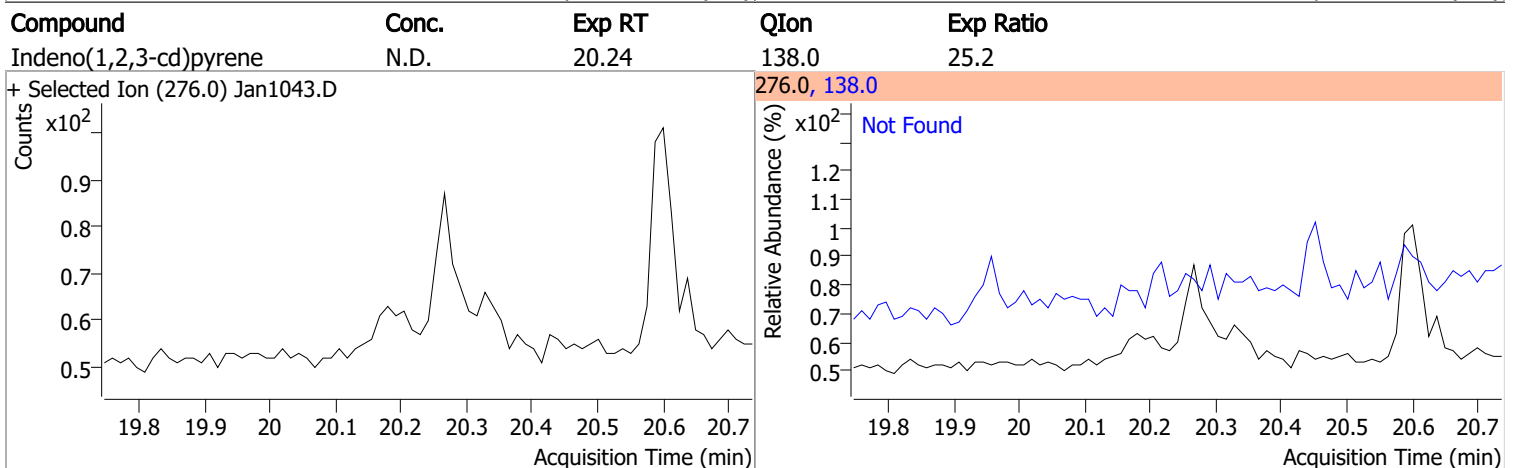


Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1044.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/11/2022 10:14:23 AM
Sample Name	B22010211-001C	Instrument	GCMS
Vial	44	Multiplier	1.00
DA Method File	011022 bna SIM 1.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 2.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.547	152.0	237238	40.0000	ng/ml	0.000
M Naphthalene-d8	6.016	136.0	670812	40.0000	ng/ml #	0.062
M Acenaphthene-d10	8.113	164.0	511124	40.0000	ng/ml #	0.100
M Phenanthrene-d10	9.805	188.0	520920	40.0000	ng/ml	0.012
M Chrysene-d12	14.751	240.0	379877	40.0000	ng/ml	-0.013
M Perylene-d12	18.512	264.0	273931	40.0000	ng/ml	-0.012
System Monitoring Compounds						
S Nitrobenzene-d5	5.168	82.0	691301	53.6869	ng/ml #m	0.000
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 1073.74%	*	
S 2-Fluorobiphenyl	7.352	172.0	1511351	59.3941	ng/ml	0.087
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1187.88%	*	
S o-Terphenyl	10.324	230.0	0		ng/ml md	0.000
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.288	244.0	735358	104.6151	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 2092.30%	*	
Target Compounds						
T Naphthalene	6.028	128.0	3041418	135.0243	ng/ml #m	59
T 2-Methylnaphthalene	6.902	141.0	7161943	551.3229	ng/ml #	64
T 1-Methylnaphthalene	7.015	141.0	6948269	578.4515	ng/ml m	91
T Acenaphthylene	7.789	152.0	0		ng/ml md	1
T Acenaphthene	7.976	154.0	0		ng/ml md	1
T Fluorene	8.748	166.0	0		ng/ml md	1
T Phenanthrene	9.830	178.0	28223	1.7810	ng/ml	90
T Anthracene	9.891	178.0	3054	0.2004	ng/ml m	96
T Fluoranthene	11.435	202.0	5600	0.3153	ng/ml	97
T Pyrene	11.818	202.0	7460	0.3936	ng/ml	95
T Benzo(a)Anthracene	14.739	228.0	3396	0.1524	ng/ml #	83
T Chrysene	14.814	228.0	3245	0.1732	ng/ml	95
T Benzo(b)fluoranthene	17.758	252.0	1748	0.1480	ng/ml m	99




Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	17.820	252.0	1087	0.0427	ng/ml	m 96
T Benzo(a)pyrene	18.400	252.0	971	0.0868	ng/ml	91
T Indeno(1,2,3-cd)pyrene	20.254	276.0	548	0.0669	ng/ml	m 92
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	20.587	276.0	874	0.0394	ng/ml	# 89




(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	53.6869	5.17	0.00	691301 (m)	54.0 128.0	45.1 28.9	21.6 21.3	40.2 39.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	135.0243	6.03	0.05	3041418 (m)	102.0 129.0	19.0 44.0	0.0 7.6	46.6 14.1




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	551.3229	6.90	0.10	7161943	142.0 115.0	98.3 71.0	103.3 36.8	191.8 68.3




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	578.4515	7.01	0.11	6948269 (m)	142.0	97.2	77.9	144.7
					115.0	64.0	44.4	82.5




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	59.3941	7.35	0.09	1511351	171.0	36.3	26.4	49.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthylene	0	0	0	0	153.0		10.2	18.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	0	0	0	0	153.0		80.3	149.2
					152.0		38.4	71.4




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene		0		0	165.0 167.0		67.5 7.9	125.3 14.6




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Phenanthrene	1.7810	9.83	0.01	28223	176.0	19.8	10.9	20.2



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Anthracene	0.2004	9.89	0.01	3054 (m)	176.0	15.1	11.6	21.6




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
o-Terphenyl		0		0	229.0 215.0		46.7 30.2	86.8 56.2




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluoranthene	0.3153	11.44	0.00	5600	101.0	10.2	8.0	14.8




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Pyrene	0.3936	11.82	0.00	7460	101.0	11.7	9.7	18.1















Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	104.6151	12.29	0.00	735358	122.0	13.5	9.6	17.9











Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)Anthracene	0.1524	14.74	0.01	3396	226.0	20.6	19.5	36.3
					229.0	33.9	16.5	30.6



Quantitation Results Report (QT Reviewed)

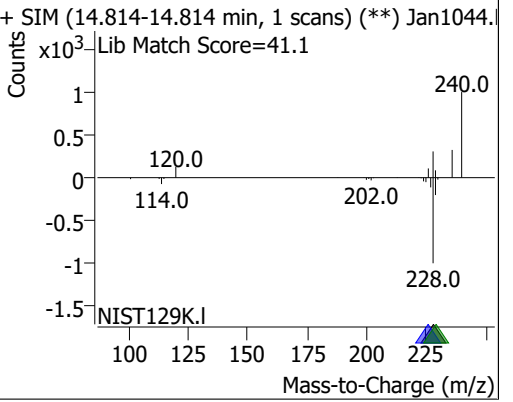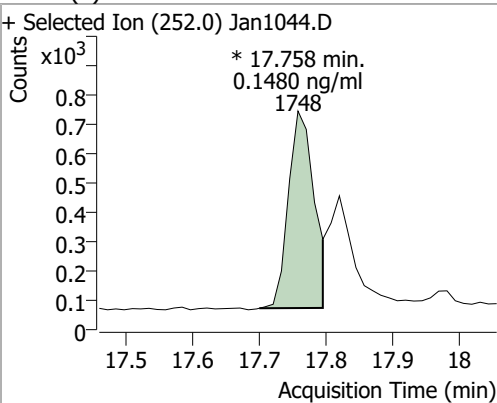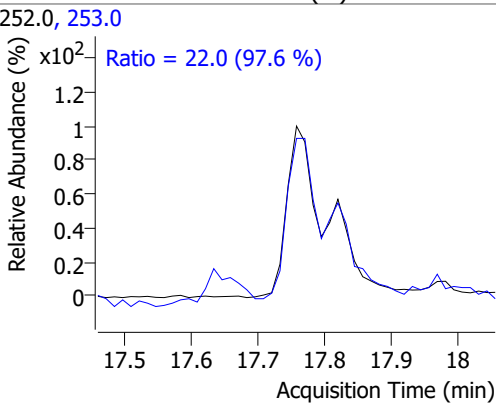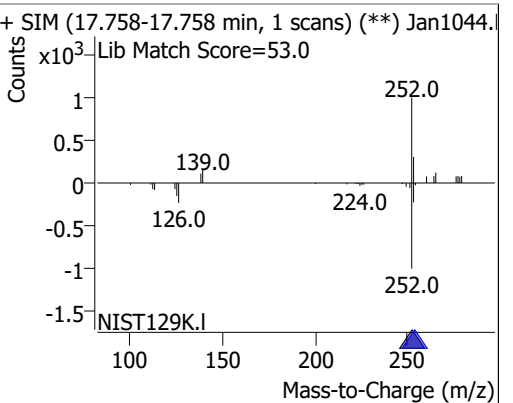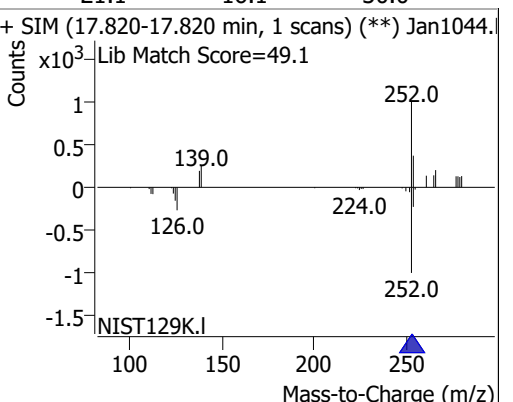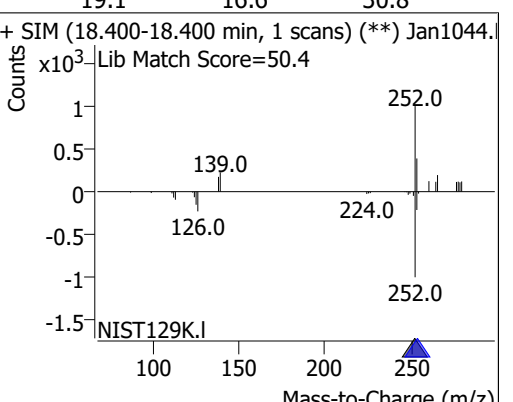Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	0.1732	14.81	-0.01	3245	226.0 229.0	29.6 25.4	22.2 15.5	41.2 28.9
+ Selected Ion (228.0) Jan1044.D 			228.0, 226.0, 229.0 			+ SIM (14.814-14.814 min, 1 scans) (**) Jan1044. Lib Match Score=41.1 		
Benzo(b)fluoranthene	0.1480	17.76	0.00	1748 (m)	253.0	22.0	15.8	29.4
+ Selected Ion (252.0) Jan1044.D 			252.0, 253.0 			+ SIM (17.758-17.758 min, 1 scans) (**) Jan1044. Lib Match Score=53.0 		
Benzo(k)fluoranthene	0.0427	17.82	0.00	1087 (m)	253.0	21.1	16.1	30.0
+ Selected Ion (252.0) Jan1044.D 			252.0, 253.0 			+ SIM (17.820-17.820 min, 1 scans) (**) Jan1044. Lib Match Score=49.1 		
Benzo(a)pyrene	0.0868	18.40	0.00	971	253.0	19.1	16.6	30.8
+ Selected Ion (252.0) Jan1044.D 			252.0, 253.0 			+ SIM (18.400-18.400 min, 1 scans) (**) Jan1044. Lib Match Score=50.4 		


Quantitation Results Report (QT Reviewed)

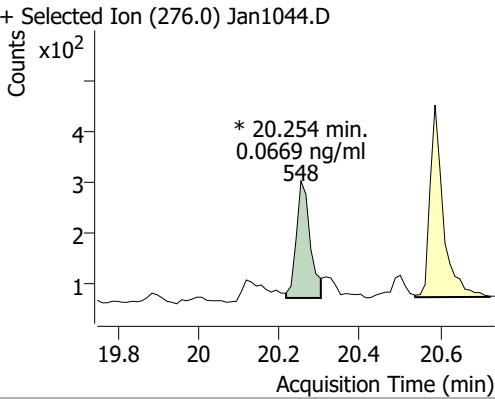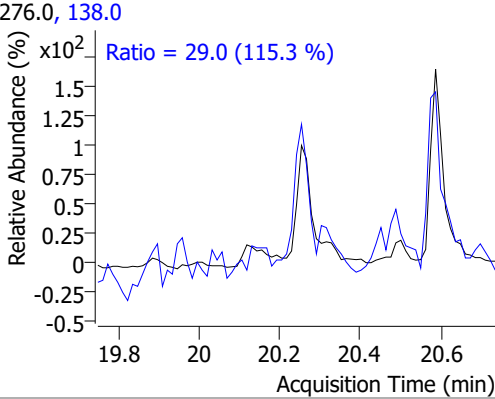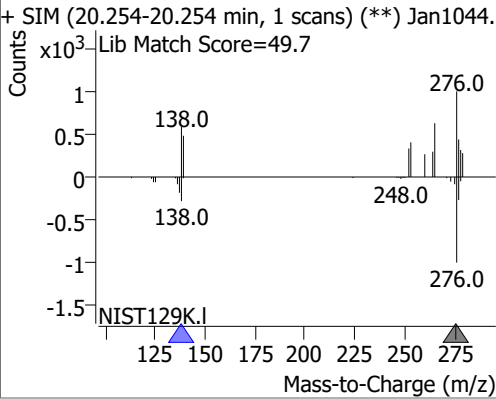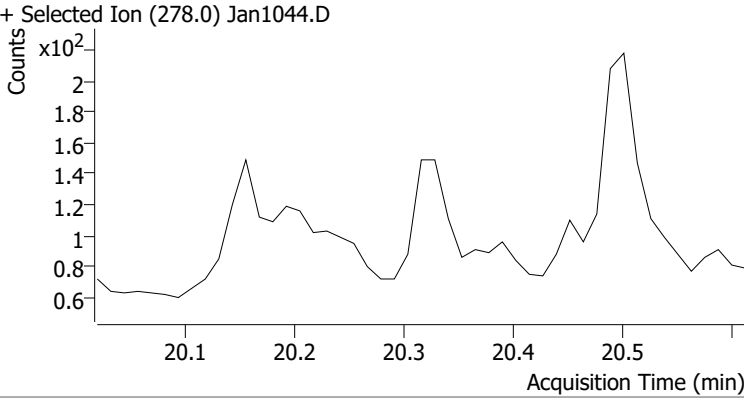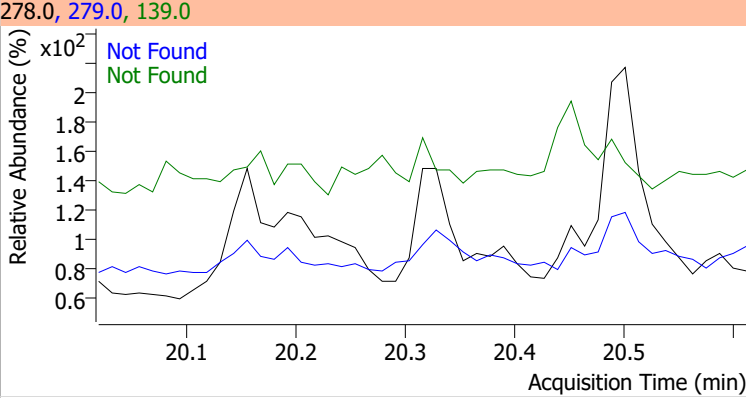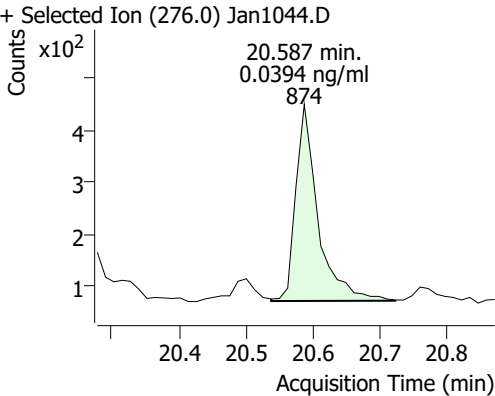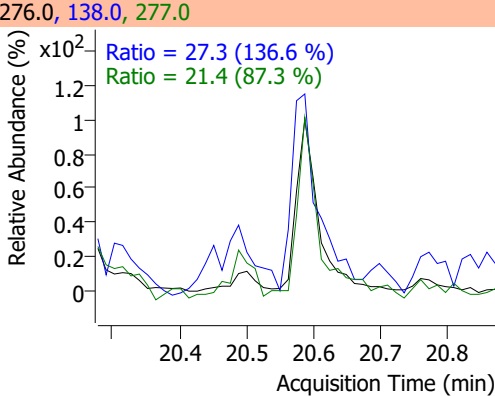Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Indeno(1,2,3-cd)pyrene	0.0669	20.25	0.01	548 (m)	138.0	29.0	17.6	32.7
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1044.D</p>  </div> <div style="width: 30%;"> <p>276.0, 138.0</p> <p>Ratio = 29.0 (115.3 %)</p>  </div> <div style="width: 30%;"> <p>+ SIM (20.254-20.254 min, 1 scans) (**) Jan1044.D</p> <p>Lib Match Score=49.7</p>  </div> </div>								
Dibenzo(a,h)anthracene	N.D.	20.32		279.0	25.9	139.0		18.3
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (278.0) Jan1044.D</p>  </div> <div style="width: 30%;"> <p>278.0, 279.0, 139.0</p> <p>Not Found Not Found</p>  </div> <div style="width: 30%;"></div> </div>								
Benzo(g,h,i)perylene	0.0394	20.59	0.01	874	277.0 138.0	21.4 27.3	17.1 14.0	31.8 25.9
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1044.D</p> <p>20.587 min. 0.0394 ng/ml</p> <p>874</p>  </div> <div style="width: 30%;"> <p>276.0, 138.0, 277.0</p> <p>Ratio = 27.3 (136.6 %) Ratio = 21.4 (87.3 %)</p>  </div> <div style="width: 30%;"> <p>+ SIM (20.587-20.587 min, 1 scans) (**) Jan1044.D</p> <p>Lib Match Score=52.3</p>  </div> </div>								

Quantitation Results Report (QT Reviewed)

Data File	Jan1045.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/11/2022 10:46:54 AM
Sample Name	B22010211-001C	Instrument	GCMS
Vial	45	Multiplier	20.00
DA Method File	011022 bna SIM 1.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 2.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	292316	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.953	136.0	495422	40.0000	ng/ml	0.000
M Acenaphthene-d10	8.026	164.0	305697	40.0000	ng/ml	0.012
M Phenanthrene-d10	9.793	188.0	638034	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	507259	40.0000	ng/ml	-0.012
M Perylene-d12	18.524	264.0	379742	40.0000	ng/ml	0.000

System Monitoring Compounds

S Nitrobenzene-d5	5.156	82.0	17944	51.9640	ng/ml	#m	-0.012
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 1039.28%		*	
S 2-Fluorobiphenyl	7.265	172.0	53200	69.9120	ng/ml		0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1398.24%		*	
S o-Terphenyl	0.000		0	N.D.			
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%			
S Terphenyl-d14	12.275	244.0	43411	92.4985	ng/ml		-0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 1849.97%		*	

Target Compounds

Compound	RT	QIon	Resp.	Conc.	Units	QValue
T Naphthalene	5.978	128.0	99745	119.9179	ng/ml	#m 62
T 2-Methylnaphthalene	6.803	141.0	358295	746.9164	ng/ml	# 64
T 1-Methylnaphthalene	6.915	141.0	233705	526.8830	ng/ml	# 85
T Acenaphthylene	7.864	152.0	0		ng/ml	md 1
T Acenaphthene	8.050	154.0	0		ng/ml	md 1
T Fluorene	8.686	166.0	0		ng/ml	md 1
T Phenanthrene	9.817	178.0	0		ng/ml	md 1
T Anthracene	9.817	178.0	0		ng/ml	md 1
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.751	228.0	0		ng/ml	md 1
T Chrysene	14.814	228.0	0		ng/ml	md 1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.401	252.0	0		ng/ml md	1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	51.9640	5.16	-0.01	17944 (m)	54.0	64.4	21.6	40.2
					128.0	51.7	21.3	39.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	119.9179	5.98	0.00	99745 (m)	102.0	21.7	0.0	46.6
					129.0	37.7	7.6	14.1




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	746.9164	6.80	0.00	358295	142.0	97.2	103.3	191.8
					115.0	70.4	36.8	68.3




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	526.8830	6.91	0.01	233705	142.0	110.9	77.9	144.7
					115.0	95.8	44.4	82.5




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	69.9120	7.26	0.00	53200	171.0	40.6	26.4	49.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthylene	0	0	0	0	153.0		10.2	18.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	0	0	0	0	153.0		80.3	149.2
					152.0		38.4	71.4




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene	0	0	0	0	165.0 167.0	7.9	67.5 7.9	125.3 14.6




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Phenanthrene	0	0	0	0	176.0	10.9	10.9	20.2



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Anthracene	0	0	0	0	176.0	11.6	11.6	21.6




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
o-Terphenyl	N.D.	10.32	229.0	66.8	215.0	43.2




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Fluoranthene	N.D.	11.44	101.0	11.4




Compound	Conc.	Exp RT	QIon	Exp Ratio
Pyrene	N.D.	11.82	101.0	13.9



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	92.4985	12.28	-0.01	43411	122.0	13.5	9.6	17.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)Anthracene		0		0	226.0		19.5	36.3
					229.0		16.5	30.6




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	0	0		0	226.0		22.2	41.2
					229.0		15.5	28.9




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene	0	0		0	253.0		16.6	30.8




Quantitation Results Report (QT Reviewed)



Quantitation Results Report (QT Reviewed)

Data File	Jan1046.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/11/2022 11:19:37 AM
Sample Name	10-Jan-22_CCV_46	Instrument	GCMS
Vial	46	Multiplier	1.00
DA Method File	011022 bna SIM 1.batch.bin	Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011022 bna SIM 2.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.522	152.0	197317	40.0000	ng/ml	-0.025
M Naphthalene-d8	5.941	136.0	370118	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	223304	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.793	188.0	459881	40.0000	ng/ml	0.000
M Chrysene-d12	14.751	240.0	358130	40.0000	ng/ml	-0.013
M Perylene-d12	18.512	264.0	255987	40.0000	ng/ml	-0.013
System Monitoring Compounds						
S Nitrobenzene-d5	5.156	82.0	7845	1.7275	ng/ml	-0.013
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 34.55%		
S 2-Fluorobiphenyl	7.264	172.0	22264	2.0027	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 40.05%		
S o-Terphenyl	10.311	230.0	16216	1.9231	ng/ml	-0.013
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = 38.46%		*
S Terphenyl-d14	12.275	244.0	14362	2.1673	ng/ml	-0.013
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 43.35%		
Target Compounds						
T Naphthalene	5.966	128.0	23500	1.8909	ng/ml	99
T 2-Methylnaphthalene	6.790	141.0	14105	1.9679	ng/ml	90
T 1-Methylnaphthalene	6.902	141.0	14935	2.2536	ng/ml	95
T Acenaphthylene	7.838	152.0	23010	1.9268	ng/ml	99
T Acenaphthene	8.050	154.0	14992	1.7267	ng/ml	97
T Fluorene	8.673	166.0	20326	2.0457	ng/ml	98
T Phenanthrene	9.817	178.0	28148	2.0170	ng/ml	91
T Anthracene	9.879	178.0	23610	2.1151	ng/ml	95
T Fluoranthene	11.435	202.0	29612	1.8890	ng/ml	99
T Pyrene	11.806	202.0	33960	1.9009	ng/ml	98
T Benzo(a)Anthracene	14.714	228.0	20842	1.9170	ng/ml	98
T Chrysene	14.813	228.0	30446	2.0687	ng/ml	98
T Benzo(b)fluoranthene	17.746	252.0	19831	1.7968	ng/ml	99


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	17.807	252.0	21176	1.8844	ng/ml	96
T Benzo(a)pyrene	18.388	252.0	14288	1.8553	ng/ml	98
T Indeno(1,2,3-cd)pyrene	20.241	276.0	13805	1.8010	ng/ml	98
T Dibenzo(a,h)anthracene	20.316	278.0	16530	1.8563	ng/ml	100
T Benzo(g,h,i)perylene	20.575	276.0	22240	2.0320	ng/ml	96


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	1.7275	5.16	-0.01	7845	54.0	32.4	21.6	40.2
					128.0	35.7	21.3	39.5















Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	1.8909	5.97	-0.01	23500	102.0	15.9	0.0	46.6
					129.0	11.3	7.6	14.1















Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	1.9679	6.79	-0.01	14105	142.0	135.9	103.3	191.8
					115.0	60.7	36.8	68.3



Quantitation Results Report (QT Reviewed)

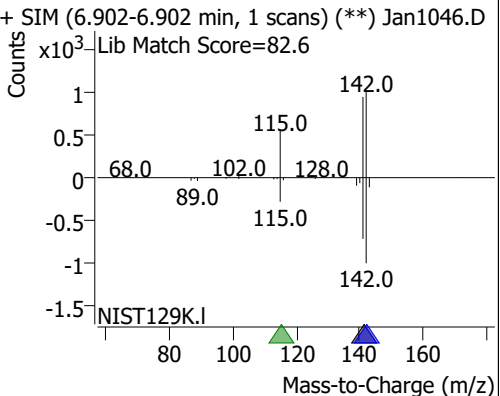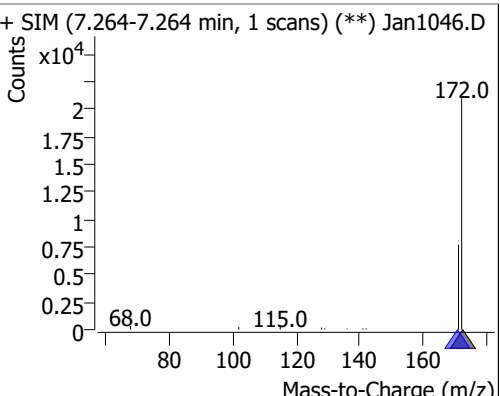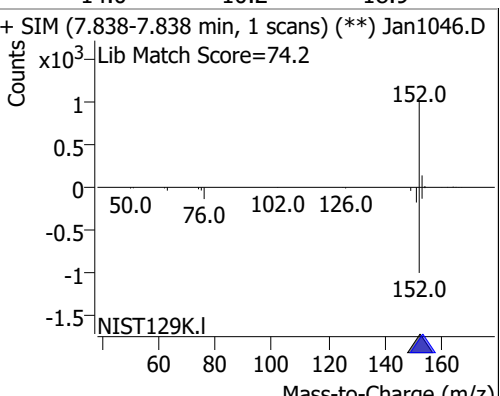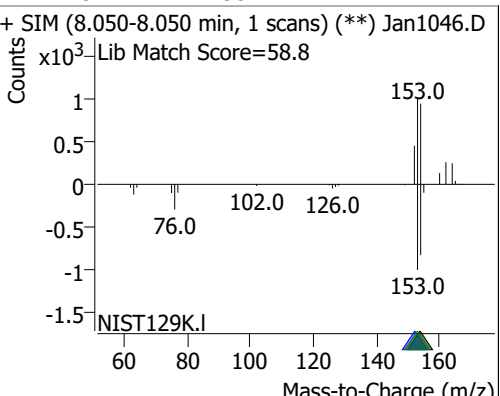
Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	2.2536	6.90	0.00	14935	142.0 115.0	116.5 58.9	77.9 44.4	144.7 82.5
+ Selected Ion (141.0) Jan1046.D 			141.0, 142.0, 115.0 			+ SIM (6.902-6.902 min, 1 scans) (**) Jan1046.D Lib Match Score=82.6 		
2-Fluorobiphenyl	2.0027	7.26	0.00	22264	171.0	36.4	26.4	49.0
+ Selected Ion (172.0) Jan1046.D 			172.0, 171.0 			+ SIM (7.264-7.264 min, 1 scans) (**) Jan1046.D Lib Match Score=82.6 		
Acenaphthylene	1.9268	7.84	0.00	23010	153.0	14.0	10.2	18.9
+ Selected Ion (152.0) Jan1046.D 			152.0, 153.0 			+ SIM (7.838-7.838 min, 1 scans) (**) Jan1046.D Lib Match Score=74.2 		
Acenaphthene	1.7267	8.05	0.00	14992	153.0 152.0	111.9 52.4	80.3 38.4	149.2 71.4
+ Selected Ion (154.0) Jan1046.D 			154.0, 152.0, 153.0 			+ SIM (8.050-8.050 min, 1 scans) (**) Jan1046.D Lib Match Score=58.8 		

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene	2.0457	8.67	-0.01	20326	165.0 167.0	98.5 13.0	67.5 7.9	125.3 14.6
+ Selected Ion (166.0) Jan1046.D 			166.0, 165.0, 167.0 			+ SIM (8.673-8.673 min, 1 scans) (**) Jan1046.D Lib Match Score=85.4 		
Phenanthrene	2.0170	9.82	0.00	28148	176.0	19.1	10.9	20.2
+ Selected Ion (178.0) Jan1046.D 			178.0, 176.0 			+ SIM (9.817-9.817 min, 1 scans) (**) Jan1046.D Lib Match Score=46.3 		
Anthracene	2.1151	9.88	0.00	23610	176.0	18.7	11.6	21.6
+ Selected Ion (178.0) Jan1046.D 			178.0, 176.0 			+ SIM (9.879-9.879 min, 1 scans) (**) Jan1046.D Lib Match Score=50.9 		
o-Terphenyl	1.9231	10.31	-0.01	16216	229.0 215.0	67.9 42.5	46.7 30.2	86.8 56.2
+ Selected Ion (230.0) Jan1046.D 			230.0, 229.0, 215.0 			+ SIM (10.311-10.311 min, 1 scans) (**) Jan1046.D Lib Match Score=76.2 		

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluoranthene	1.8890	11.44	0.00	29612	101.0	11.8	8.0	14.8




Pyrene	1.9009	11.81	-0.01	33960	101.0	13.3	9.7	18.1
--------	--------	-------	-------	-------	-------	------	-----	------



Terphenyl-d14	2.1673	12.28	-0.01	14362	122.0	14.3	9.6	17.9
---------------	--------	-------	-------	-------	-------	------	-----	------




Benzo(a)Anthracene	1.9170	14.71	-0.01	20842	226.0	27.2	19.5	36.3
					229.0	24.4	16.5	30.6




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	2.0687	14.81	-0.01	30446	226.0	31.0	22.2	41.2
					229.0	21.2	15.5	28.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(b)fluoranthene	1.7968	17.75	-0.01	19831	253.0	22.0	15.8	29.4












Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(k)fluoranthene	1.8844	17.81	-0.01	21176	253.0	25.1	16.1	30.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene	1.8553	18.39	-0.01	14288	253.0	24.9	16.6	30.8



Quantitation Results Report (QT Reviewed)

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Indeno(1,2,3-cd)pyrene	1.8010	20.24	0.00	13805	138.0	24.2	17.6	32.7
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1046.D</p>  </div> <div style="width: 30%;"> <p>276.0, 138.0</p> <p>Ratio = 24.2 (96.2 %)</p>  </div> <div style="width: 30%;"> <p>+ SIM (20.241-20.241 min, 1 scans) (**) Jan1046.</p> <p>Lib Match Score=76.3</p>  </div> </div>								
Dibenzo(a,h)anthracene	1.8563	20.32	0.00	16530	279.0	26.1	18.1	33.6
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (278.0) Jan1046.D</p>  </div> <div style="width: 30%;"> <p>278.0, 279.0, 139.0</p> <p>Ratio = 26.1 (100.8 %)</p> <p>Ratio = 18.5 (101.1 %)</p>  </div> <div style="width: 30%;"> <p>+ SIM (20.316-20.316 min, 1 scans) (**) Jan1046.</p> <p>Lib Match Score=75.9</p>  </div> </div>								
Benzo(g,h,i)perylene	2.0320	20.58	0.00	22240	277.0	22.1	17.1	31.8
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1046.D</p>  </div> <div style="width: 30%;"> <p>276.0, 138.0, 277.0</p> <p>Ratio = 21.2 (106.3 %)</p> <p>Ratio = 22.1 (90.1 %)</p>  </div> <div style="width: 30%;"> <p>+ SIM (20.575-20.575 min, 1 scans) (**) Jan1046.</p> <p>Lib Match Score=76.4</p>  </div> </div>								

Continuing Calibration Report

Batch Name \\MASSHUNTER\Org\Data\SV5975.I\sh011022\2 e8270d bna SIM\QuantResults\011022 bna SIM 2.batch.bin
Method File \\MASSHUNTER\Org\Data\SV5975.I\sh011022\1 e8270d bna SIM\011022 bna SIM 1.batch.bin
Daily CC \\MASSHUNTER\Org\Data\SV5975.I\sh011022\2 e8270d bna SIM\Jan1025.D

Level name	Injection Time	Calibration Files
7	12/28/2021 5:30:40 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2802.D
6	12/28/2021 6:03:21 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2803.D
5	12/28/2021 6:35:53 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2804.D
4	12/28/2021 7:08:33 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2805.D
3	12/28/2021 7:41:06 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2806.D
2	12/28/2021 8:13:46 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2807.D
1	12/28/2021 8:46:23 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2808.D
CCV	1/10/2022 11:59:38 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh011022\2 e8270d bna SIM\Jan1025.D <=====

ISTD Compound:	Avg Resp	Mid Resp	CC Resp	Area%	A/M
1,4-Dichlorobenzene-d4	305106	324694	224889	69.26	M
Naphthalene-d8	572584	593232	419423	70.70	M
Acenaphthene-d10	319385	333337	262799	78.84	M
Phenanthrene-d10	689765	735690	554012	75.31	M
Chrysene-d12	520451	540068	439231	81.33	M
Perylene-d12	336551	351697	309386	87.97	M

Target Compound	AvgRF/R2	CC RF	Exp. Conc	Calc. Conc	%Dev	Area%	Curve Fit
1,4-Dichlorobenzene-d4	-----ISTD-----						
Nitrobenzene-d5	0.9996	0.7996	2.00	1.74	13.17	62.25	Quadratic
Naphthalene-d8	-----ISTD-----						
Naphthalene	1.3431	1.2989	2.00	1.93	-3.30	71.85	Avg RF
2-Methylnaphthalene	0.7746	0.8118	2.00	2.10	4.80	79.11	Avg RF
1-Methylnaphthalene	0.7163	0.8442	2.00	2.36	17.86	90.73	Avg RF
Acenaphthene-d10	-----ISTD-----						
2-Fluorobiphenyl	1.9914	1.9371	2.00	1.95	-2.73	84.72	Avg RF
Acenaphthylene	2.1392	2.0636	2.00	1.93	-3.54	84.49	Avg RF
Acenaphthene	1.5553	1.3364	2.00	1.72	-14.07	72.75	Avg RF
Fluorene	1.7797	1.7969	2.00	2.02	0.96	86.03	Avg RF
Phenanthrene-d10	-----ISTD-----						
Phenanthrene	0.9990	1.2199	2.00	2.01	-0.49	78.96	Quadratic
Anthracene	0.9997	0.9950	2.00	2.05	-2.53	78.66	Quadratic
o-Terphenyl	0.7334	0.6705	2.00	1.83	-8.58	78.58	Avg RF
Fluoranthene	1.3635	1.3040	2.00	1.91	-4.36	80.66	Avg RF
Chrysene-d12	-----ISTD-----						
Pyrene	1.9954	1.8433	2.00	1.85	-7.62	82.43	Avg RF
Terphenyl-d14	0.7402	0.7512	2.00	2.03	1.50	89.77	Avg RF
Benzo(a)Anthracene	0.9978	1.1652	2.00	1.92	4.04	80.16	Quadratic
Chrysene	0.9966	1.6379	2.00	1.99	0.38	83.03	Quadratic
Perylene-d12	-----ISTD-----						
Benzo(b)fluoranthene	1.7246	1.4706	2.00	1.71	-14.73	77.84	Avg RF
Benzo(k)fluoranthene	0.9999	1.7568	2.00	2.00	0.09	85.75	Quadratic
Benzo(a)pyrene	0.9996	1.1319	2.00	1.88	5.98	82.50	Quadratic
Indeno(1,2,3-cd)pyrene	1.1977	1.0083	2.00	1.68	-15.82	80.74	Avg RF
Dibenzo(a,h)anthracene	1.3915	1.2486	2.00	1.79	-10.27	85.16	Avg RF
Benzo(g,h,i)perylene	0.9993	1.6587	2.00	1.94	2.84	84.23	Quadratic

A -- against Average; M -- against Mid Point; P -- against Previous CC in the Method;

Continuing Calibration Report

Batch Name \\MASSHUNTER\Org\Data\SV5975.I\sh011022\2 e8270d bna SIM\QuantResults\011022 bna SIM 2.batch.bin
Method File \\MASSHUNTER\Org\Data\SV5975.I\sh011022\1 e8270d bna SIM\011022 bna SIM 1.batch.bin
Daily CC \\MASSHUNTER\Org\Data\SV5975.I\sh011022\2 e8270d bna SIM\Jan1046.D

Level name	Injection Time	Calibration Files
7	12/28/2021 5:30:40 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2802.D
6	12/28/2021 6:03:21 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2803.D
5	12/28/2021 6:35:53 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2804.D
4	12/28/2021 7:08:33 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2805.D
3	12/28/2021 7:41:06 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2806.D
2	12/28/2021 8:13:46 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2807.D
1	12/28/2021 8:46:23 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2808.D
CCV	1/11/2022 11:19:37 AM	\\MASSHUNTER\Org\Data\SV5975.I\sh011022\2 e8270d bna SIM\Jan1046.D <=====

ISTD Compound:	Avg Resp	Mid Resp	CC Resp	Area%	A/M
1,4-Dichlorobenzene-d4	305106	324694	224889	69.26	M
Naphthalene-d8	572584	593232	419423	70.70	M
Acenaphthene-d10	319385	333337	262799	78.84	M
Phenanthrene-d10	689765	735690	554012	75.31	M
Chrysene-d12	520451	540068	439231	81.33	M
Perylene-d12	336551	351697	309386	87.97	M

Target Compound	AvgRF/R2	CC RF	Exp. Conc	Calc. Conc	%Dev	Area%	Curve Fit
1,4-Dichlorobenzene-d4	-----ISTD-----						
Nitrobenzene-d5	0.9996	0.7996	2.00	1.74	13.17	62.25	Quadratic
Naphthalene-d8	-----ISTD-----						
Naphthalene	1.3431	1.2989	2.00	1.93	-3.30	71.85	Avg RF
2-Methylnaphthalene	0.7746	0.8118	2.00	2.10	4.80	79.11	Avg RF
1-Methylnaphthalene	0.7163	0.8442	2.00	2.36	17.86	90.73	Avg RF
Acenaphthene-d10	-----ISTD-----						
2-Fluorobiphenyl	1.9914	1.9371	2.00	1.95	-2.73	84.72	Avg RF
Acenaphthylene	2.1392	2.0636	2.00	1.93	-3.54	84.49	Avg RF
Acenaphthene	1.5553	1.3364	2.00	1.72	-14.07	72.75	Avg RF
Fluorene	1.7797	1.7969	2.00	2.02	0.96	86.03	Avg RF
Phenanthrene-d10	-----ISTD-----						
Phenanthrene	0.9990	1.2199	2.00	2.01	-0.49	78.96	Quadratic
Anthracene	0.9997	0.9950	2.00	2.05	-2.53	78.66	Quadratic
o-Terphenyl	0.7334	0.6705	2.00	1.83	-8.58	78.58	Avg RF
Fluoranthene	1.3635	1.3040	2.00	1.91	-4.36	80.66	Avg RF
Chrysene-d12	-----ISTD-----						
Pyrene	1.9954	1.8433	2.00	1.85	-7.62	82.43	Avg RF
Terphenyl-d14	0.7402	0.7512	2.00	2.03	1.50	89.77	Avg RF
Benzo(a)Anthracene	0.9978	1.1652	2.00	1.92	4.04	80.16	Quadratic
Chrysene	0.9966	1.6379	2.00	1.99	0.38	83.03	Quadratic
Perylene-d12	-----ISTD-----						
Benzo(b)fluoranthene	1.7246	1.4706	2.00	1.71	-14.73	77.84	Avg RF
Benzo(k)fluoranthene	0.9999	1.7568	2.00	2.00	0.09	85.75	Quadratic
Benzo(a)pyrene	0.9996	1.1319	2.00	1.88	5.98	82.50	Quadratic
Indeno(1,2,3-cd)pyrene	1.1977	1.0083	2.00	1.68	-15.82	80.74	Avg RF
Dibenzo(a,h)anthracene	1.3915	1.2486	2.00	1.79	-10.27	85.16	Avg RF
Benzo(g,h,i)perylene	0.9993	1.6587	2.00	1.94	2.84	84.23	Quadratic

A -- against Average; M -- against Mid Point; P -- against Previous CC in the Method;

Audit Trail report

Batch name and path: \\MASSHUNTER\Org\Data\SV5975.I\sh011022\2 e8270d bna SIM\QuantResults\011022 bna SIM 2.batch.bin
Quant batch version: 10.0
Quant reporting version: 10.0

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdNewBatchTable	BL2000\jheine	1/11/2022 8:46:32 AM	Create new batch \\MASSHUNTER\Org\Data\SV5975.I\sh011022\2 e8270d bna SIM\011022 bna SIM 2.batch.bin			✓	
CmdImportSamplesFromWorklist	BL2000\jheine	1/11/2022 8:47:11 AM	Add samples from worklist: \\MASSHUNTER\Org\Data\SV5975.I\sh011022\2 e8270d bna SIM\Jan1040.D, \\MASSHUNTER\Org\Data\SV5975.I\sh011022\2 e8270d bna SIM\Jan1039.D, \\MASSHUNTER\Org\Data\SV5975.I\sh011022\2 e8270d bna SIM\Jan1038.D, \\MASSHUNTER\Org\Data\SV5975.I\sh011022\2 e8270d bna SIM\Jan1037.D, \\MASSHUNTER\Org\Data\SV5975.I\sh011022\2 e8270d bna SIM\Jan1036.D, \\MASSHUNTER\Org\Data\SV5975.I\sh011022\2 e8270d bna SIM\Jan1035.D, \\MASSHUNTER\Org\Data\SV5975.I\sh011022\2 e8270d bna SIM\Jan1035.D, \\MASSHUNTER\Org\Data\SV5975.I\sh011022\2 e8270d bna SIM\Jan1034.D, \\MASSHUNTER\Org\Data\SV5975.I\sh011022\2 e8270d bna SIM\Jan1033.D, \\MASSHUNTER\Org\Data\SV5975.I\sh011022\2 e8270d bna SIM\Jan1032.D, \\MASSHUNTER\Org\Data\SV5975.I\sh011022\2 e8270d bna SIM\Jan1031.D, \\MASSHUNTER\Org\Data\SV5975.I\sh011022\2 e8270d bna SIM\Jan1030.D, \\MASSHUNTER\Org\Data\SV5975.I\sh011022\2 e8270d bna SIM\Jan1029.D, \\MASSHUNTER\Org\Data\SV5975.I\sh011022\2 e8270d bna SIM\Jan1028.D, \\MASSHUNTER\Org\Data\SV5975.I\sh011022\2 e8270d bna SIM\Jan1027.D, \\MASSHUNTER\Org\Data\SV5975.I\sh011022\2 e8270d bna SIM\Jan1026.D, \\MASSHUNTER\Org\Data\SV5975.I\sh011022\2 e8270d bna SIM\Jan1025.D, \\MASSHUNTER\Org\Data\SV5975.I\sh011022\2 e8270d bna SIM\Jan1024.D			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:47:18 AM	Set SampleType = TuneCheck for sample Jan1024.D; previous value = Sample			✓	
CmdStartMethodEditing	BL2000\jheine	1/11/2022 8:48:13 AM	Start method editing			✓	
CmdImportMethodFromBatch	BL2000\jheine	1/11/2022 8:48:15 AM	Import method from batch \\MASSHUNTER\Org\Data\SV5975.I\sh011022\1 e8270d bna SIM\011022 bna SIM 1.batch.bin			✓	
CmdApplyMethodToAllSamples	BL2000\jheine	1/11/2022 8:48:21 AM	Apply method to all samples			✓	
CmdMethodClear	BL2000\jheine	1/11/2022 8:48:21 AM	Clear method			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdEndMethodEditing	BL2000\jheine	1/11/2022 8:48:22 AM	End method editing			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:48:31 AM	Set SampleType = CC for sample Jan1025.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:48:34 AM	Set LevelName = CCV for sample Jan1025.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:48:37 AM	Set SampleType = Matrix for sample Jan1033.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:48:43 AM	Set MatrixSpikeGroup = B22010141-001C for sample Jan1031.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:48:44 AM	Set MatrixSpikeGroup = B22010141-001C for sample Jan1033.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 8:48:47 AM	Set SampleInformation = MatrixA for sample Jan1033.D; previous value =			✓	
CmdQuantitate	BL2000\jheine	1/11/2022 8:48:56 AM	Quantitate all compounds in all samples			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/11/2022 8:49:15 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1025.D, from x, y = 5.953, 564 to 6.084, 104, result = 2610; previous integration is from x, y = 5.897, 83 to 6.084, 104 and previous response = 8593.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:49:16 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1025.D to y = 104, new integration is from x, y = 5.953, 104 to 6.084, 104 and new response = 4415; previous integration is from x, y = 5.953, 564 to 6.084, 104 and previous response = 2610.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/11/2022 8:49:34 AM	Manually integrate qualifier 152.0 of compound Acenaphthene in sample Jan1025.D from x, y = 8.025, 1262 to 8.100, 5003; result = -4162			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/11/2022 8:49:35 AM	Snap baseline for qualifier 152.0 of compound Acenaphthene in sample Jan1025.D from x = 8.025 to x = 8.100, new integration is from x, y = 8.025, 133 to 8.100, 221 and new response = 9096; previous integration is from x, y = 8.025, 1262 to 8.100, 5003 and previous response = -4162.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:49:36 AM	Drop baseline for qualifier 152.0 of compound Acenaphthene in sample Jan1025.D to y = 133, new integration is from x, y = 8.025, 133 to 8.100, 133 and new response = 9293; previous integration is from x, y = 8.025, 133 to 8.100, 221 and previous response = 9096.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:50:19 AM	Manually integrate compound Benzo(a)pyrene in sample Jan1026.D, from x, y = 18.376, 101 to 18.437, 223, result = -318; previous integration is from x, y = 18.462, 59 to 18.648, 61 and previous response = 1891.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/11/2022 8:50:20 AM	Snap baseline for compound Benzo(a)pyrene in sample Jan1026.D, from x = 18.376 to x = 18.437, new integration is from x, y = 18.376, 57 to 18.437, 67 and new response = 53; previous integration is from x, y = 18.376, 101 to 18.437, 223 and previous response = -318.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:50:21 AM	Drop baseline for compound Benzo(a)pyrene in sample Jan1026.D to y = 57, new integration is from x, y = 18.376, 57 to 18.437, 57 and new response = 71; previous integration is from x, y = 18.376, 57 to 18.437, 67 and previous response = 53.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:50:22 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1026.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:50:28 AM	Manually integrate compound Acenaphthene in sample Jan1026.D, from x, y = 8.038, 325 to 8.100, 66, result = -303; previous integration is from x, y = 7.988, 66 to 8.100, 66 and previous response = 1546.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:50:30 AM	Drop baseline for compound Acenaphthene in sample Jan1026.D to y = 66, new integration is from x, y = 8.038, 66 to 8.100, 66 and new response = 183; previous integration is from x, y = 8.038, 325 to 8.100, 66 and previous response = -303.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:50:32 AM	Zero out primary peak of compound Acenaphthene in sample Jan1026.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:50:34 AM	Zero out primary peak of compound Chrysene in sample Jan1026.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:50:35 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1026.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:50:47 AM	Zero out primary peak of compound Fluorene in sample Jan1027.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:50:50 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1027.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:50:55 AM	Zero out primary peak of compound Acenaphthene in sample Jan1027.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:50:56 AM	Zero out primary peak of compound Chrysene in sample Jan1027.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:50:59 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1027.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:51:14 AM	Manually integrate compound Benzo(a)pyrene in sample Jan1028.D, from x, y = 18.376, 123 to 18.437, 210, result = -315; previous integration is from x, y = 18.476, 68 to 18.660, 76 and previous response = 2092.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/11/2022 8:51:16 AM	Snap baseline for compound Benzo(a)pyrene in sample Jan1028.D, from x = 18.376 to x = 18.437, new integration is from x, y = 18.376, 60 to 18.437, 67 and new response = 67; previous integration is from x, y = 18.376, 123 to 18.437, 210 and previous response = -315.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:51:16 AM	Drop baseline for compound Benzo(a)pyrene in sample Jan1028.D to y = 60, new integration is from x, y = 18.376, 60 to 18.437, 60 and new response = 80; previous integration is from x, y = 18.376, 60 to 18.437, 67 and previous response = 67.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:51:18 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1028.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:51:21 AM	Zero out primary peak of compound Acenaphthene in sample Jan1028.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:51:23 AM	Zero out primary peak of compound Chrysene in sample Jan1028.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:51:24 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1028.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:51:37 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1029.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:51:40 AM	Zero out primary peak of compound Acenaphthene in sample Jan1029.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:51:42 AM	Zero out primary peak of compound Chrysene in sample Jan1029.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:51:43 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1029.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:51:54 AM	Manually integrate compound Benzo(a)pyrene in sample Jan1030.D, from x, y = 18.388, 89 to 18.438, 234, result = -238; previous integration is from x, y = 18.465, 65 to 18.660, 67 and previous response = 1899.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/11/2022 8:51:55 AM	Snap baseline for compound Benzo(a)pyrene in sample Jan1030.D, from x = 18.388 to x = 18.438, new integration is from x, y = 18.388, 67 to 18.438, 63 and new response = 47; previous integration is from x, y = 18.388, 89 to 18.438, 234 and previous response = -238.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:51:56 AM	Drop baseline for compound Benzo(a)pyrene in sample Jan1030.D to y = 63, new integration is from x, y = 18.388, 63 to 18.438, 63 and new response = 53; previous integration is from x, y = 18.388, 67 to 18.438, 63 and previous response = 47.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:51:58 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1030.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:52:04 AM	Manually integrate compound Acenaphthene in sample Jan1030.D, from x, y = 8.038, 89 to 8.088, 66, result = 111; previous integration is from x, y = 7.988, 66 to 8.088, 66 and previous response = 1536.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:52:05 AM	Drop baseline for compound Acenaphthene in sample Jan1030.D to y = 66, new integration is from x, y = 8.038, 66 to 8.088, 66 and new response = 145; previous integration is from x, y = 8.038, 89 to 8.088, 66 and previous response = 111.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:52:06 AM	Zero out primary peak of compound Acenaphthene in sample Jan1030.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:52:12 AM	Manually integrate compound Chrysene in sample Jan1030.D, from x, y = 14.801, 94 to 14.888, 54, result = 137; previous integration is from x, y = 14.684, 54 to 14.888, 54 and previous response = 2096.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:52:14 AM	Drop baseline for compound Chrysene in sample Jan1030.D to y = 54, new integration is from x, y = 14.801, 54 to 14.888, 54 and new response = 241; previous integration is from x, y = 14.801, 94 to 14.888, 54 and previous response = 137.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:52:15 AM	Zero out primary peak of compound Chrysene in sample Jan1030.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:52:18 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1030.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:52:32 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1031.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:52:36 AM	Zero out primary peak of compound Acenaphthene in sample Jan1031.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:52:38 AM	Zero out primary peak of compound Chrysene in sample Jan1031.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:52:39 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1031.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:52:51 AM	Manually integrate compound Benzo(a)pyrene in sample Jan1032.D, from x, y = 18.388, 99 to 18.438, 183, result = -176; previous integration is from x, y = 18.476, 63 to 18.660, 64 and previous response = 2046.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/11/2022 8:52:52 AM	Snap baseline for compound Benzo(a)pyrene in sample Jan1032.D, from x = 18.388 to x = 18.438, new integration is from x, y = 18.388, 69 to 18.438, 64 and new response = 46; previous integration is from x, y = 18.388, 99 to 18.438, 183 and previous response = -176.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:52:53 AM	Drop baseline for compound Benzo(a)pyrene in sample Jan1032.D to y = 64, new integration is from x, y = 18.388, 64 to 18.438, 64 and new response = 53; previous integration is from x, y = 18.388, 69 to 18.438, 64 and previous response = 46.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:52:54 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1032.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:53:00 AM	Manually integrate compound Acenaphthene in sample Jan1032.D, from x, y = 8.038, 134 to 8.100, 66, result = 48; previous integration is from x, y = 7.988, 66 to 8.100, 66 and previous response = 1673.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:53:02 AM	Drop baseline for compound Acenaphthene in sample Jan1032.D to y = 66, new integration is from x, y = 8.038, 66 to 8.100, 66 and new response = 176; previous integration is from x, y = 8.038, 134 to 8.100, 66 and previous response = 48.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:53:03 AM	Zero out primary peak of compound Acenaphthene in sample Jan1032.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:53:06 AM	Zero out primary peak of compound Chrysene in sample Jan1032.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:53:07 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1032.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/11/2022 8:53:23 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1033.D, from x, y = 5.953, 970 to 6.053, 88, result = 5926; previous integration is from x, y = 5.894, 88 to 6.053, 88 and previous response = 12947.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:53:25 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1033.D to y = 88, new integration is from x, y = 5.953, 88 to 6.053, 88 and new response = 8568; previous integration is from x, y = 5.953, 970 to 6.053, 88 and previous response = 5926.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/11/2022 8:53:35 AM	Manually integrate qualifier 142.0 of compound 2-Methylnaphthalene in sample Jan1033.D, from x, y = 6.765, 67 to 6.815, 1836, result = 31049; previous integration is from x, y = 6.765, 67 to 6.877, 67 and previous response = 48322.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:53:36 AM	Drop baseline for qualifier 142.0 of compound 2-Methylnaphthalene in sample Jan1033.D to y = 67, new integration is from x, y = 6.765, 67 to 6.815, 67 and new response = 33701; previous integration is from x, y = 6.765, 67 to 6.815, 1836 and previous response = 31049.			✓	
CmdClearManualIntegration	BL2000\jheine	1/11/2022 8:53:45 AM	Clear manual integration of qualifier 142.0 for compound 2-Methylnaphthalene in sample Jan1033.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:54:35 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1034.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:54:39 AM	Zero out primary peak of compound Acenaphthene in sample Jan1034.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:54:40 AM	Zero out primary peak of compound Chrysene in sample Jan1034.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:54:42 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1034.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:54:59 AM	Manually integrate compound Benzo(a)pyrene in sample Jan1035.D, from x, y = 18.376, 79 to 18.450, 148, result = -173; previous integration is from x, y = 18.475, 63 to 18.648, 64 and previous response = 1928.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/11/2022 8:55:00 AM	Snap baseline for compound Benzo(a)pyrene in sample Jan1035.D, from x = 18.376 to x = 18.450, new integration is from x, y = 18.376, 60 to 18.450, 60 and new response = 66; previous integration is from x, y = 18.376, 79 to 18.450, 148 and previous response = -173.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:55:01 AM	Drop baseline for compound Benzo(a)pyrene in sample Jan1035.D to y = 60, new integration is from x, y = 18.376, 60 to 18.450, 60 and new response = 66; previous integration is from x, y = 18.376, 60 to 18.450, 60 and previous response = 66.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:55:03 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1035.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:55:09 AM	Manually integrate compound Acenaphthene in sample Jan1035.D, from x, y = 8.038, 136 to 8.100, 65, result = 41; previous integration is from x, y = 7.976, 65 to 8.100, 65 and previous response = 1635.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:55:11 AM	Drop baseline for compound Acenaphthene in sample Jan1035.D to y = 65, new integration is from x, y = 8.038, 65 to 8.100, 65 and new response = 173; previous integration is from x, y = 8.038, 136 to 8.100, 65 and previous response = 41.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:55:12 AM	Zero out primary peak of compound Acenaphthene in sample Jan1035.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:55:17 AM	Manually integrate compound Chrysene in sample Jan1035.D, from x, y = 14.789, 97 to 14.913, 52, result = 187; previous integration is from x, y = 14.669, 51 to 14.913, 52 and previous response = 2248.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:55:19 AM	Drop baseline for compound Chrysene in sample Jan1035.D to y = 52, new integration is from x, y = 14.789, 52 to 14.913, 52 and new response = 353; previous integration is from x, y = 14.789, 97 to 14.913, 52 and previous response = 187.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:55:20 AM	Zero out primary peak of compound Chrysene in sample Jan1035.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:55:24 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1035.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:55:35 AM	Manually integrate compound Benzo(a)pyrene in sample Jan1036.D, from x, y = 18.376, 94 to 18.438, 192, result = -240; previous integration is from x, y = 18.462, 65 to 18.648, 76 and previous response = 2165.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/11/2022 8:55:36 AM	Snap baseline for compound Benzo(a)pyrene in sample Jan1036.D, from x = 18.376 to x = 18.438, new integration is from x, y = 18.376, 64 to 18.438, 62 and new response = 56; previous integration is from x, y = 18.376, 94 to 18.438, 192 and previous response = -240.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:55:36 AM	Drop baseline for compound Benzo(a)pyrene in sample Jan1036.D to y = 62, new integration is from x, y = 18.376, 62 to 18.438, 62 and new response = 60; previous integration is from x, y = 18.376, 64 to 18.438, 62 and previous response = 56.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:55:38 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1036.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:55:44 AM	Manually integrate compound Acenaphthene in sample Jan1036.D, from x, y = 8.038, 147 to 8.088, 76, result = 26; previous integration is from x, y = 7.976, 76 to 8.088, 76 and previous response = 1778.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:55:46 AM	Drop baseline for compound Acenaphthene in sample Jan1036.D to y = 76, new integration is from x, y = 8.038, 76 to 8.088, 76 and new response = 132; previous integration is from x, y = 8.038, 147 to 8.088, 76 and previous response = 26.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:55:47 AM	Zero out primary peak of compound Acenaphthene in sample Jan1036.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:55:53 AM	Manually integrate compound Chrysene in sample Jan1036.D, from x, y = 14.801, 156 to 14.863, 253, result = -347; previous integration is from x, y = 14.679, 56 to 14.839, 56 and previous response = 2271.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/11/2022 8:55:55 AM	Snap baseline for compound Chrysene in sample Jan1036.D, from x = 14.801 to x = 14.863, new integration is from x, y = 14.801, 122 to 14.863, 77 and new response = 46; previous integration is from x, y = 14.801, 156 to 14.863, 253 and previous response = -347.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:55:55 AM	Drop baseline for compound Chrysene in sample Jan1036.D to y = 77, new integration is from x, y = 14.801, 77 to 14.863, 77 and new response = 130; previous integration is from x, y = 14.801, 122 to 14.863, 77 and previous response = 46.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:55:57 AM	Zero out primary peak of compound Chrysene in sample Jan1036.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:56:00 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1036.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:56:18 AM	Manually integrate compound Benzo(a)pyrene in sample Jan1037.D, from x, y = 18.376, 88 to 18.450, 165, result = -212; previous integration is from x, y = 18.476, 71 to 18.648, 73 and previous response = 2033.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/11/2022 8:56:19 AM	Snap baseline for compound Benzo(a)pyrene in sample Jan1037.D, from x = 18.376 to x = 18.450, new integration is from x, y = 18.376, 55 to 18.450, 61 and new response = 93; previous integration is from x, y = 18.376, 88 to 18.450, 165 and previous response = -212.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:56:19 AM	Drop baseline for compound Benzo(a)pyrene in sample Jan1037.D to y = 55, new integration is from x, y = 18.376, 55 to 18.450, 55 and new response = 107; previous integration is from x, y = 18.376, 55 to 18.450, 61 and previous response = 93.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:56:22 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1037.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:56:29 AM	Manually integrate compound Acenaphthene in sample Jan1037.D, from x, y = 8.038, 110 to 8.088, 67, result = 93; previous integration is from x, y = 7.987, 67 to 8.088, 67 and previous response = 1770.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:56:30 AM	Drop baseline for compound Acenaphthene in sample Jan1037.D to y = 67, new integration is from x, y = 8.038, 67 to 8.088, 67 and new response = 158; previous integration is from x, y = 8.038, 110 to 8.088, 67 and previous response = 93.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:56:31 AM	Zero out primary peak of compound Acenaphthene in sample Jan1037.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:56:37 AM	Manually integrate compound Chrysene in sample Jan1037.D, from x, y = 14.801, 173 to 14.876, 183, result = -302; previous integration is from x, y = 14.677, 53 to 14.838, 53 and previous response = 2283.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/11/2022 8:56:39 AM	Snap baseline for compound Chrysene in sample Jan1037.D, from x = 14.801 to x = 14.876, new integration is from x, y = 14.801, 134 to 14.876, 71 and new response = 38; previous integration is from x, y = 14.801, 173 to 14.876, 183 and previous response = -302.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:56:40 AM	Drop baseline for compound Chrysene in sample Jan1037.D to y = 71, new integration is from x, y = 14.801, 71 to 14.876, 71 and new response = 179; previous integration is from x, y = 14.801, 134 to 14.876, 71 and previous response = 38.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:56:42 AM	Zero out primary peak of compound Chrysene in sample Jan1037.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:56:43 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1037.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:57:00 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1038.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:57:06 AM	Manually integrate compound Acenaphthene in sample Jan1038.D, from x, y = 8.038, 147 to 8.075, 81, result = 26; previous integration is from x, y = 7.988, 82 to 8.075, 81 and previous response = 1562.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:57:08 AM	Drop baseline for compound Acenaphthene in sample Jan1038.D to y = 81, new integration is from x, y = 8.038, 81 to 8.075, 81 and new response = 100; previous integration is from x, y = 8.038, 147 to 8.075, 81 and previous response = 26.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:57:09 AM	Zero out primary peak of compound Acenaphthene in sample Jan1038.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:57:16 AM	Manually integrate compound Chrysene in sample Jan1038.D, from x, y = 14.789, 183 to 14.876, 241, result = -542; previous integration is from x, y = 14.684, 56 to 14.838, 56 and previous response = 2260.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/11/2022 8:57:17 AM	Snap baseline for compound Chrysene in sample Jan1038.D, from x = 14.789 to x = 14.876, new integration is from x, y = 14.789, 130 to 14.876, 74 and new response = 34; previous integration is from x, y = 14.789, 183 to 14.876, 241 and previous response = -542.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:57:18 AM	Drop baseline for compound Chrysene in sample Jan1038.D to y = 74, new integration is from x, y = 14.789, 74 to 14.876, 74 and new response = 180; previous integration is from x, y = 14.789, 130 to 14.876, 74 and previous response = 34.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:57:19 AM	Zero out primary peak of compound Chrysene in sample Jan1038.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:57:21 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1038.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:57:38 AM	Manually integrate compound Benzo(a)pyrene in sample Jan1039.D, from x, y = 18.388, 117 to 18.450, 172, result = -241; previous integration is from x, y = 18.462, 61 to 18.660, 71 and previous response = 2044.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/11/2022 8:57:39 AM	Snap baseline for compound Benzo(a)pyrene in sample Jan1039.D, from x = 18.388 to x = 18.450, new integration is from x, y = 18.388, 66 to 18.450, 63 and new response = 54; previous integration is from x, y = 18.388, 117 to 18.450, 172 and previous response = -241.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:57:40 AM	Drop baseline for compound Benzo(a)pyrene in sample Jan1039.D to y = 63, new integration is from x, y = 18.388, 63 to 18.450, 63 and new response = 60; previous integration is from x, y = 18.388, 66 to 18.450, 63 and previous response = 54.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:57:42 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1039.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:57:47 AM	Manually integrate compound Acenaphthene in sample Jan1039.D, from x, y = 8.038, 92 to 8.088, 67, result = 116; previous integration is from x, y = 7.988, 67 to 8.088, 67 and previous response = 1579.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:57:48 AM	Drop baseline for compound Acenaphthene in sample Jan1039.D to y = 67, new integration is from x, y = 8.038, 67 to 8.088, 67 and new response = 154; previous integration is from x, y = 8.038, 92 to 8.088, 67 and previous response = 116.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:57:50 AM	Zero out primary peak of compound Acenaphthene in sample Jan1039.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:57:56 AM	Manually integrate compound Chrysene in sample Jan1039.D, from x, y = 14.789, 180 to 14.888, 207, result = -508; previous integration is from x, y = 14.680, 54 to 14.838, 54 and previous response = 2247.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/11/2022 8:57:57 AM	Snap baseline for compound Chrysene in sample Jan1039.D, from x = 14.789 to x = 14.888, new integration is from x, y = 14.789, 128 to 14.888, 73 and new response = 49; previous integration is from x, y = 14.789, 180 to 14.888, 207 and previous response = -508.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:57:58 AM	Drop baseline for compound Chrysene in sample Jan1039.D to y = 73, new integration is from x, y = 14.789, 73 to 14.888, 73 and new response = 213; previous integration is from x, y = 14.789, 128 to 14.888, 73 and previous response = 49.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:58:00 AM	Zero out primary peak of compound Chrysene in sample Jan1039.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:58:03 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1039.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:58:21 AM	Zero out primary peak of compound Fluorene in sample Jan1040.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:58:25 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1040.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:58:30 AM	Manually integrate compound Acenaphthene in sample Jan1040.D, from x, y = 8.038, 214 to 8.075, 268, result = -182; previous integration is from x, y = 7.988, 73 to 8.100, 73 and previous response = 1775.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/11/2022 8:58:31 AM	Snap baseline for compound Acenaphthene in sample Jan1040.D, from x = 8.038 to x = 8.075, new integration is from x, y = 8.038, 152 to 8.075, 102 and new response = 74; previous integration is from x, y = 8.038, 214 to 8.075, 268 and previous response = -182.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:58:31 AM	Drop baseline for compound Acenaphthene in sample Jan1040.D to y = 102, new integration is from x, y = 8.038, 102 to 8.075, 102 and new response = 130; previous integration is from x, y = 8.038, 152 to 8.075, 102 and previous response = 74.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:58:33 AM	Zero out primary peak of compound Acenaphthene in sample Jan1040.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 8:58:40 AM	Manually integrate compound Chrysene in sample Jan1040.D, from x, y = 14.789, 175 to 14.876, 226, result = -483; previous integration is from x, y = 14.679, 55 to 14.838, 55 and previous response = 2269.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/11/2022 8:58:41 AM	Snap baseline for compound Chrysene in sample Jan1040.D, from x = 14.789 to x = 14.876, new integration is from x, y = 14.789, 118 to 14.876, 74 and new response = 61; previous integration is from x, y = 14.789, 175 to 14.876, 226 and previous response = -483.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 8:58:42 AM	Drop baseline for compound Chrysene in sample Jan1040.D to y = 74, new integration is from x, y = 14.789, 74 to 14.876, 74 and new response = 176; previous integration is from x, y = 14.789, 118 to 14.876, 74 and previous response = 61.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:58:44 AM	Zero out primary peak of compound Chrysene in sample Jan1040.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 8:58:47 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1040.D			✓	
CmdSaveBatchTable	BL2000\jheine	1/11/2022 8:58:58 AM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh011022\2 e8270d bna SIM\QuantResults\011022 bna SIM 2.batch.bin			✓	
CmdSaveBatchTable	BL2000\jheine	1/11/2022 9:01:55 AM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh011022\2 e8270d bna SIM\QuantResults\011022 bna SIM 2.batch.bin			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 9:02:01 AM	Set SampleApproved = True for sample Jan1024.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 9:02:02 AM	Set SampleApproved = True for sample Jan1025.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 9:02:03 AM	Set SampleApproved = True for sample Jan1026.D; previous value = False			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 9:02:06 AM	Set SampleApproved = True for sample Jan1027.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 9:02:07 AM	Set SampleApproved = True for sample Jan1028.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 9:02:08 AM	Set SampleApproved = True for sample Jan1029.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 9:02:09 AM	Set SampleApproved = True for sample Jan1030.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 9:02:11 AM	Set SampleApproved = True for sample Jan1031.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 9:02:12 AM	Set SampleApproved = True for sample Jan1032.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 9:02:14 AM	Set SampleApproved = True for sample Jan1033.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 9:02:16 AM	Set SampleApproved = True for sample Jan1034.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 9:02:18 AM	Set SampleApproved = True for sample Jan1035.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 9:02:20 AM	Set SampleApproved = True for sample Jan1036.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 9:02:21 AM	Set SampleApproved = True for sample Jan1037.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 9:02:22 AM	Set SampleApproved = True for sample Jan1038.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 9:02:24 AM	Set SampleApproved = True for sample Jan1039.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 9:02:27 AM	Set SampleApproved = True for sample Jan1040.D; previous value = False			✓	
CmdSaveBatchTable	BL2000\jheine	1/11/2022 9:02:48 AM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\2 e8270d bna SIM\QuantResults\011022 bna SIM 2.batch.bin			✓	
CmdSaveBatchTable	BL2000\jheine	1/11/2022 9:09:02 AM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\2 e8270d bna SIM\QuantResults\011022 bna SIM 2.batch.bin			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdOpenBatchTable	BL2000\jheine	1/11/2022 11:43:57 AM	Open batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\2 e8270d bna SIM\011022 bna SIM 2.batch.bin			✓	
CmdImportSamplesFromWorklist	BL2000\jheine	1/11/2022 11:44:31 AM	Add samples from worklist: \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\2 e8270d bna SIM\Jan1046.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\2 e8270d bna SIM\Jan1045.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\2 e8270d bna SIM\Jan1044.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\2 e8270d bna SIM\Jan1043.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\2 e8270d bna SIM\Jan1042.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\2 e8270d bna SIM\Jan1041.D			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 11:45:00 AM	Set SampleType = CC for sample Jan1046.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/11/2022 11:45:04 AM	Set LevelName = CCV for sample Jan1046.D; previous value =			✓	
CmdQuantitate	BL2000\jheine	1/11/2022 11:45:11 AM	Quantitate all compounds in all samples			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/11/2022 11:45:32 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1046.D, from x, y = 5.953, 2110 to 6.041, 1883, result = -6176; previous integration is from x, y = 5.897, 78 to 6.178, 78 and previous response = 7766.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/11/2022 11:45:33 AM	Snap baseline for qualifier 102.0 of compound Naphthalene in sample Jan1046.D from x = 5.953 to x = 6.041, new integration is from x, y = 5.953, 1163 to 6.041, 108 and new response = 963; previous integration is from x, y = 5.953, 2110 to 6.041, 1883 and previous response = -6176.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 11:45:34 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1046.D to y = 108, new integration is from x, y = 5.953, 108 to 6.041, 108 and new response = 3730; previous integration is from x, y = 5.953, 1163 to 6.041, 108 and previous response = 963.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/11/2022 11:45:46 AM	Manually integrate qualifier 152.0 of compound Acenaphthene in sample Jan1046.D from x, y = 8.025, 2174 to 8.113, 3642; result = -6687			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/11/2022 11:45:47 AM	Snap baseline for qualifier 152.0 of compound Acenaphthene in sample Jan1046.D from x = 8.025 to x = 8.113, new integration is from x, y = 8.025, 129 to 8.113, 171 and new response = 7750; previous integration is from x, y = 8.025, 2174 to 8.113, 3642 and previous response = -6687.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 11:45:48 AM	Drop baseline for qualifier 152.0 of compound Acenaphthene in sample Jan1046.D to y = 129, new integration is from x, y = 8.025, 129 to 8.113, 129 and new response = 7860; previous integration is from x, y = 8.025, 129 to 8.113, 171 and previous response = 7750.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 11:47:23 AM	Manually integrate compound Benzo(a)pyrene in sample Jan1041.D, from x, y = 18.376, 59 to 18.450, 59, result = 74; previous integration is from x, y = 18.469, 62 to 18.660, 70 and previous response = 1837.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 11:47:25 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1041.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 11:47:29 AM	Manually integrate compound Acenaphthene in sample Jan1041.D, from x, y = 8.038, 259 to 8.100, 66, result = -196; previous integration is from x, y = 7.976, 66 to 8.100, 66 and previous response = 1557.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 11:47:31 AM	Drop baseline for compound Acenaphthene in sample Jan1041.D to y = 66, new integration is from x, y = 8.038, 66 to 8.100, 66 and new response = 165; previous integration is from x, y = 8.038, 259 to 8.100, 66 and previous response = -196.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 11:47:32 AM	Zero out primary peak of compound Acenaphthene in sample Jan1041.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 11:47:39 AM	Manually integrate compound Chrysene in sample Jan1041.D, from x, y = 14.789, 166 to 14.901, 169, result = -453; previous integration is from x, y = 14.677, 53 to 14.901, 53 and previous response = 2089.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/11/2022 11:47:40 AM	Snap baseline for compound Chrysene in sample Jan1041.D, from x = 14.789 to x = 14.901, new integration is from x, y = 14.789, 128 to 14.901, 68 and new response = 12; previous integration is from x, y = 14.789, 166 to 14.901, 169 and previous response = -453.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 11:47:41 AM	Drop baseline for compound Chrysene in sample Jan1041.D to y = 68, new integration is from x, y = 14.789, 68 to 14.901, 68 and new response = 214; previous integration is from x, y = 14.789, 128 to 14.901, 68 and previous response = 12.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 11:47:42 AM	Zero out primary peak of compound Chrysene in sample Jan1041.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 11:47:45 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1041.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 11:47:59 AM	Manually integrate compound Fluorene in sample Jan1042.D, from x, y = 8.661, 67 to 8.723, 78, result = 75; previous integration is from x, y = 8.961, 73 to 9.122, 74 and previous response = 9108.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 11:48:00 AM	Zero out primary peak of compound Fluorene in sample Jan1042.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 11:48:07 AM	Manually integrate compound Benzo(a)pyrene in sample Jan1042.D, from x, y = 18.388, 67 to 18.425, 65, result = 20; previous integration is from x, y = 18.475, 66 to 18.660, 67 and previous response = 1964.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 11:48:08 AM	Drop baseline for compound Benzo(a)pyrene in sample Jan1042.D to y = 65, new integration is from x, y = 18.388, 65 to 18.425, 65 and new response = 22; previous integration is from x, y = 18.388, 67 to 18.425, 65 and previous response = 20.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 11:48:09 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1042.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 11:48:14 AM	Manually integrate compound Acenaphthene in sample Jan1042.D, from x, y = 8.038, 290 to 8.088, 83, result = -205; previous integration is from x, y = 7.989, 83 to 8.088, 83 and previous response = 1537.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 11:48:15 AM	Drop baseline for compound Acenaphthene in sample Jan1042.D to y = 83, new integration is from x, y = 8.038, 83 to 8.088, 83 and new response = 104; previous integration is from x, y = 8.038, 290 to 8.088, 83 and previous response = -205.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 11:48:18 AM	Zero out primary peak of compound Acenaphthene in sample Jan1042.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 11:48:21 AM	Zero out primary peak of compound Chrysene in sample Jan1042.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdZeroOutPeak	BL2000\jheine	1/11/2022 11:48:22 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1042.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 11:49:01 AM	Manually integrate compound Benzo(a)pyrene in sample Jan1043.D, from x, y = 18.376, 57 to 18.425, 68, result = 55; previous integration is from x, y = 18.475, 64 to 18.611, 70 and previous response = 2112.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 11:49:02 AM	Drop baseline for compound Benzo(a)pyrene in sample Jan1043.D to y = 57, new integration is from x, y = 18.376, 57 to 18.425, 57 and new response = 71; previous integration is from x, y = 18.376, 57 to 18.425, 68 and previous response = 55.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 11:49:03 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1043.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 11:49:11 AM	Manually integrate compound Acenaphthene in sample Jan1043.D, from x, y = 8.038, 290 to 8.100, 66, result = -248; previous integration is from x, y = 7.985, 66 to 8.100, 66 and previous response = 1793.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 11:49:12 AM	Drop baseline for compound Acenaphthene in sample Jan1043.D to y = 66, new integration is from x, y = 8.038, 66 to 8.100, 66 and new response = 172; previous integration is from x, y = 8.038, 290 to 8.100, 66 and previous response = -248.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 11:49:13 AM	Zero out primary peak of compound Acenaphthene in sample Jan1043.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 11:49:16 AM	Zero out primary peak of compound Chrysene in sample Jan1043.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 11:49:17 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1043.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 11:49:38 AM	Manually integrate compound Nitrobenzene-d5 in sample Jan1044.D, from x, y = 5.131, 173952 to 5.205, 226529, result = 573660; previous integration is from x, y = 5.094, 233 to 5.205, 238 and previous response = 1778920.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 11:49:40 AM	Drop baseline for compound Nitrobenzene-d5 in sample Jan1044.D to y = 173952, new integration is from x, y = 5.131, 173952 to 5.205, 173952 and new response = 691301; previous integration is from x, y = 5.131, 173952 to 5.205, 226529 and previous response = 573660.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/11/2022 11:49:46 AM	Manually integrate qualifier 54.0 of compound Nitrobenzene-d5 in sample Jan1044.D, from x, y = 5.143, 69664 to 5.218, 80878, result = 286437; previous integration is from x, y = 5.094, 312 to 5.268, 327 and previous response = 1135276.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 11:49:47 AM	Drop baseline for qualifier 54.0 of compound Nitrobenzene-d5 in sample Jan1044.D to y = 69664, new integration is from x, y = 5.143, 69664 to 5.218, 69664 and new response = 311529; previous integration is from x, y = 5.143, 69664 to 5.218, 80878 and previous response = 286437.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/11/2022 11:49:51 AM	Manually integrate qualifier 128.0 of compound Nitrobenzene-d5 in sample Jan1044.D, from x, y = 5.143, 9990 to 5.243, 628, result = 171691; previous integration is from x, y = 5.094, 628 to 5.243, 628 and previous response = 231198.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 11:49:52 AM	Drop baseline for qualifier 128.0 of compound Nitrobenzene-d5 in sample Jan1044.D to y = 628, new integration is from x, y = 5.143, 628 to 5.243, 628 and new response = 199623; previous integration is from x, y = 5.143, 9990 to 5.243, 628 and previous response = 171691.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/11/2022 11:49:57 AM	Set UserAnnotation = BA for compound Nitrobenzene-d5 in sample Jan1044.D; previous value =			✓	
CmdSelectPeak	BL2000\jheine	1/11/2022 11:50:01 AM	Select peak for compound Naphthalene in sample Jan1044.D			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/11/2022 11:50:07 AM	Manually integrate qualifier 129.0 of compound Naphthalene in sample Jan1044.D, from x, y = 5.966, 10600 to 6.078, 53955, result = 1193275; previous integration is from x, y = 5.999, 73017 to 6.078, 88327 and previous response = 957907.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 11:50:08 AM	Drop baseline for qualifier 129.0 of compound Naphthalene in sample Jan1044.D to y = 10600, new integration is from x, y = 5.966, 10600 to 6.078, 10600 and new response = 1339468; previous integration is from x, y = 5.966, 10600 to 6.078, 53955 and previous response = 1193275.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/11/2022 11:50:12 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1044.D, from x, y = 5.978, 13223 to 6.078, 28684, result = 531860; previous integration is from x, y = 6.000, 52812 to 6.078, 52812 and previous response = 364531.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 11:50:13 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1044.D to y = 13223, new integration is from x, y = 5.978, 13223 to 6.078, 13223 and new response = 578203; previous integration is from x, y = 5.978, 13223 to 6.078, 28684 and previous response = 531860.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/11/2022 11:50:23 AM	Manually integrate qualifier 115.0 of compound 2-Methylnaphthalene in sample Jan1044.D, from x, y = 6.852, 266905 to 6.965, 373, result = 4185642; previous integration is from x, y = 6.790, 373 to 6.965, 373 and previous response = 7272615.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 11:50:25 AM	Drop baseline for qualifier 115.0 of compound 2-Methylnaphthalene in sample Jan1044.D to y = 373, new integration is from x, y = 6.852, 373 to 6.965, 373 and new response = 5084390; previous integration is from x, y = 6.852, 266905 to 6.965, 373 and previous response = 4185642.			✓	
CmdSelectPeak	BL2000\jheine	1/11/2022 11:50:32 AM	Select peak for compound 1-Methylnaphthalene in sample Jan1044.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 11:50:36 AM	Manually integrate compound 1-Methylnaphthalene in sample Jan1044.D, from x, y = 6.952, 53329 to 7.052, 770267, result = 4799604; previous integration is from x, y = 6.952, 53329 to 7.127, 53329 and previous response = 7534052.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 11:50:37 AM	Drop baseline for compound 1-Methylnaphthalene in sample Jan1044.D to y = 53329, new integration is from x, y = 6.952, 53329 to 7.052, 53329 and new response = 6948269; previous integration is from x, y = 6.952, 53329 to 7.052, 770267 and previous response = 4799604.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 11:53:21 AM	Zero out primary peak of compound Acenaphthylene in sample Jan1044.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 11:53:32 AM	Zero out primary peak of compound Acenaphthene in sample Jan1044.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/11/2022 11:53:43 AM	Manually integrate qualifier 167.0 of compound Fluorene in sample Jan1044.D, from x, y = 8.736, 63007 to 8.773, 18611, result = 23311; previous integration is from x, y = 8.712, 19801 to 8.773, 18611 and previous response = 87503.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 11:53:44 AM	Drop baseline for qualifier 167.0 of compound Fluorene in sample Jan1044.D to y = 18611, new integration is from x, y = 8.736, 18611 to 8.773, 18611 and new response = 73123; previous integration is from x, y = 8.736, 63007 to 8.773, 18611 and previous response = 23311.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 11:53:52 AM	Manually integrate compound Fluorene in sample Jan1044.D, from x, y = 8.698, 6976 to 8.773, 9452, result = 189856; previous integration is from x, y = 8.717, 16502 to 8.767, 15166 and previous response = 161054.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 11:53:53 AM	Drop baseline for compound Fluorene in sample Jan1044.D to y = 6976, new integration is from x, y = 8.698, 6976 to 8.773, 6976 and new response = 195411; previous integration is from x, y = 8.698, 6976 to 8.773, 9452 and previous response = 189856.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 11:54:19 AM	Zero out primary peak of compound Fluorene in sample Jan1044.D			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/11/2022 11:54:25 AM	Manually integrate qualifier 176.0 of compound Phenanthrene in sample Jan1044.D, from x, y = 9.799, 636 to 9.867, 1713, result = 3404; previous integration is from x, y = 9.799, 636 to 9.916, 592 and previous response = 6067.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 11:54:26 AM	Drop baseline for qualifier 176.0 of compound Phenanthrene in sample Jan1044.D to y = 636, new integration is from x, y = 9.799, 636 to 9.867, 636 and new response = 5583; previous integration is from x, y = 9.799, 636 to 9.867, 1713 and previous response = 3404.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 11:55:53 AM	Manually integrate compound Anthracene in sample Jan1044.D, from x, y = 9.867, 1923 to 9.916, 2862, result = -1512; previous integration is from x, y = 9.867, 481 to 9.953, 470 and previous response = 6095.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateS napBaseline	BL2000\jheine	1/11/2022 11:55:54 AM	Snap baseline for compound Anthracene in sample Jan1044.D, from x = 9.867 to x = 9.916, new integration is from x, y = 9.867, 1241 to 9.916, 1322 and new response = 1781; previous integration is from x, y = 9.867, 1923 to 9.916, 2862 and previous response = -1512.			✓	
CmdManuallyIntegrate DropBaseline	BL2000\jheine	1/11/2022 11:55:55 AM	Drop baseline for compound Anthracene in sample Jan1044.D to y = 1241, new integration is from x, y = 9.867, 1241 to 9.916, 1241 and new response = 1901; previous integration is from x, y = 9.867, 1241 to 9.916, 1322 and previous response = 1781.			✓	
CmdManuallyIntegrate QualifierPeak	BL2000\jheine	1/11/2022 11:55:59 AM	Manually integrate qualifier 176.0 of compound Anthracene in sample Jan1044.D from x, y = 9.867, 1583 to 9.916, 592; result = -1007			✓	
CmdManuallyIntegrate DropBaseline	BL2000\jheine	1/11/2022 11:56:00 AM	Drop baseline for qualifier 176.0 of compound Anthracene in sample Jan1044.D to y = 592, new integration is from x, y = 9.867, 592 to 9.916, 592 and new response = 461; previous integration is from x, y = 9.867, 1583 to 9.916, 592 and previous response = -1007.			✓	
CmdManuallyIntegrateP eak	BL2000\jheine	1/11/2022 11:56:14 AM	Manually integrate compound Anthracene in sample Jan1044.D, from x, y = 9.867, 1639 to 9.916, 852, result = 1888; previous integration is from x, y = 9.867, 1241 to 9.916, 1241 and previous response = 1901.			✓	
CmdManuallyIntegrate DropBaseline	BL2000\jheine	1/11/2022 11:56:15 AM	Drop baseline for compound Anthracene in sample Jan1044.D to y = 852, new integration is from x, y = 9.867, 852 to 9.916, 852 and new response = 3054; previous integration is from x, y = 9.867, 1639 to 9.916, 852 and previous response = 1888.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 11:56:29 AM	Zero out primary peak of compound o-Terphenyl in sample Jan1044.D			✓	
CmdManuallyIntegrateS plit	BL2000\jheine	1/11/2022 11:57:43 AM	Split qualifier 101.0 of compound Pyrene in sample Jan1044.D and keep left peak, new integration is from x, y = 11.783, 148.391960549491 to 11.855, 146.110811011221 and new response = 874, previous integration is from x, y = 11.783, 148 to 11.967, 143 and previous response = 1071.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateSplit	BL2000\jheine	1/11/2022 11:57:57 AM	Split peak for compound Benzo(b)fluoranthene in sample Jan1044.D and keep left peak, new integration is from x, y = 17.700, 71.2834427121837 to 17.795, 72.3450597347011 and new response = 1748, previous integration is from x, y = 17.700, 71 to 17.931, 74 and previous response = 2833.			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	1/11/2022 11:58:00 AM	Split qualifier 253.0 of compound Benzo(b)fluoranthene in sample Jan1044.D and keep left peak, new integration is from x, y = 17.712, 84.2038889232711 to 17.795, 86.2556661294094 and new response = 385, previous integration is from x, y = 17.712, 84 to 17.910, 89 and previous response = 614.			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	1/11/2022 11:58:04 AM	Split peak for compound Benzo(k)fluoranthene in sample Jan1044.D and keep right peak, new integration is from x, y = 17.795, 72.3450597347011 to 17.931, 73.8665920298526 and new response = 1087, previous integration is from x, y = 17.700, 71 to 17.931, 74 and previous response = 2833.			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	1/11/2022 11:58:09 AM	Split qualifier 253.0 of compound Benzo(k)fluoranthene in sample Jan1044.D and keep right peak, new integration is from x, y = 17.795, 86.2556661294094 to 17.910, 89.0799300849458 and new response = 230, previous integration is from x, y = 17.712, 84 to 17.910, 89 and previous response = 614.			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	1/11/2022 11:58:18 AM	Split peak for compound Indeno(1,2,3-cd)pyrene in sample Jan1044.D and keep left peak, new integration is from x, y = 20.217, 70.5173400493621 to 20.316, 71.2631913932721 and new response = 576, previous integration is from x, y = 20.217, 71 to 20.413, 72 and previous response = 657.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 11:58:21 AM	Manually integrate compound Indeno(1,2,3-cd)pyrene in sample Jan1044.D, from x, y = 20.217, 71 to 20.303, 88, result = 503; previous integration is from x, y = 20.217, 71 to 20.316, 71 and previous response = 576.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 11:58:23 AM	Drop baseline for compound Indeno(1,2,3-cd)pyrene in sample Jan1044.D to y = 71, new integration is from x, y = 20.217, 71 to 20.303, 71 and new response = 548; previous integration is from x, y = 20.217, 71 to 20.303, 88 and previous response = 503.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/11/2022 11:58:24 AM	Set UserAnnotation = CO for compound Indeno(1,2,3-cd)pyrene in sample Jan1044.D; previous value =			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	1/11/2022 11:58:27 AM	Split qualifier 138.0 of compound Indeno(1,2,3-cd)pyrene in sample Jan1044.D and keep left peak, new integration is from x, y = 20.204, 107.551036872801 to 20.303, 109.250715423691 and new response = 163, previous integration is from x, y = 20.204, 108 to 20.358, 110 and previous response = 192.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/11/2022 11:58:31 AM	Manually integrate qualifier 138.0 of compound Indeno(1,2,3-cd)pyrene in sample Jan1044.D, from x, y = 20.204, 108 to 20.291, 135, result = 87; previous integration is from x, y = 20.204, 108 to 20.303, 109 and previous response = 163.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 11:58:32 AM	Drop baseline for qualifier 138.0 of compound Indeno(1,2,3-cd)pyrene in sample Jan1044.D to y = 108, new integration is from x, y = 20.204, 108 to 20.291, 108 and new response = 159; previous integration is from x, y = 20.204, 108 to 20.291, 135 and previous response = 87.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/11/2022 11:58:42 AM	Manually integrate qualifier 138.0 of compound Benzo(g,h,i)perylene in sample Jan1044.D from x, y = 20.550, 105 to 20.662, 110; result = 222			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 11:58:44 AM	Drop baseline for qualifier 138.0 of compound Benzo(g,h,i)perylene in sample Jan1044.D to y = 105, new integration is from x, y = 20.550, 105 to 20.662, 105 and new response = 238; previous integration is from x, y = 20.550, 105 to 20.662, 110 and previous response = 222.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/11/2022 11:58:49 AM	Manually integrate qualifier 277.0 of compound Benzo(g,h,i)perylene in sample Jan1044.D from x, y = 20.563, 74 to 20.686, 74; result = 187			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 12:25:07 PM	Manually integrate compound Nitrobenzene-d5 in sample Jan1045.D, from x, y = 5.106, 9657 to 5.156, 11316, result = 15470; previous integration is from x, y = 5.044, 256 to 5.230, 267 and previous response = 158950.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 12:25:08 PM	Drop baseline for compound Nitrobenzene-d5 in sample Jan1045.D to y = 9657, new integration is from x, y = 5.106, 9657 to 5.156, 9657 and new response = 17944; previous integration is from x, y = 5.106, 9657 to 5.156, 11316 and previous response = 15470.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/11/2022 12:25:12 PM	Manually integrate qualifier 54.0 of compound Nitrobenzene-d5 in sample Jan1045.D, from x, y = 5.118, 564 to 5.168, 3920, result = 15952; previous integration is from x, y = 5.118, 564 to 5.218, 564 and previous response = 40036.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/11/2022 12:25:13 PM	Snap baseline for qualifier 54.0 of compound Nitrobenzene-d5 in sample Jan1045.D from x = 5.118 to x = 5.168, new integration is from x, y = 5.118, 3714 to 5.168, 6399 and new response = 7556; previous integration is from x, y = 5.118, 564 to 5.168, 3920 and previous response = 15952.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 12:25:14 PM	Drop baseline for qualifier 54.0 of compound Nitrobenzene-d5 in sample Jan1045.D to y = 3714, new integration is from x, y = 5.118, 3714 to 5.168, 3714 and new response = 11561; previous integration is from x, y = 5.118, 3714 to 5.168, 6399 and previous response = 7556.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 12:25:28 PM	Manually integrate compound Naphthalene in sample Jan1045.D, from x, y = 5.953, 2709 to 6.016, 194, result = 95033; previous integration is from x, y = 5.916, 194 to 6.016, 194 and previous response = 108922.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 12:25:29 PM	Drop baseline for compound Naphthalene in sample Jan1045.D to y = 194, new integration is from x, y = 5.953, 194 to 6.016, 194 and new response = 99745; previous integration is from x, y = 5.953, 2709 to 6.016, 194 and previous response = 95033.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/11/2022 12:25:32 PM	Set UserAnnotation = CO for compound Naphthalene in sample Jan1045.D; previous value =			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/11/2022 12:25:38 PM	Manually integrate qualifier 129.0 of compound Naphthalene in sample Jan1045.D, from x, y = 5.953, 560 to 5.991, 1124, result = 36981; previous integration is from x, y = 5.953, 4423 to 5.991, 4423 and previous response = 19447.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 12:25:40 PM	Drop baseline for qualifier 129.0 of compound Naphthalene in sample Jan1045.D to y = 560, new integration is from x, y = 5.953, 560 to 5.991, 560 and new response = 37615; previous integration is from x, y = 5.953, 560 to 5.991, 1124 and previous response = 36981.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/11/2022 12:25:47 PM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1045.D, from x, y = 5.953, 7478 to 5.991, 780, result = 14131; previous integration is from x, y = 5.931, 2504 to 6.006, 2504 and previous response = 20785.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 12:25:49 PM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1045.D to y = 780, new integration is from x, y = 5.953, 780 to 5.991, 780 and new response = 21660; previous integration is from x, y = 5.953, 7478 to 5.991, 780 and previous response = 14131.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 12:26:18 PM	Manually integrate compound Acenaphthene in sample Jan1045.D, from x, y = 8.038, 1241 to 8.063, 1587, result = 3191; previous integration is from x, y = 8.038, 1241 to 8.163, 1152 and previous response = 12680.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 12:26:19 PM	Drop baseline for compound Acenaphthene in sample Jan1045.D to y = 1241, new integration is from x, y = 8.038, 1241 to 8.063, 1241 and new response = 3448; previous integration is from x, y = 8.038, 1241 to 8.063, 1587 and previous response = 3191.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/11/2022 12:26:23 PM	Manually integrate qualifier 152.0 of compound Acenaphthene in sample Jan1045.D, from x, y = 8.028, 2079 to 8.063, 3068, result = 14967; previous integration is from x, y = 8.028, 2079 to 8.138, 1953 and previous response = 28092.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 12:26:24 PM	Drop baseline for qualifier 152.0 of compound Acenaphthene in sample Jan1045.D to y = 2079, new integration is from x, y = 8.028, 2079 to 8.063, 2079 and new response = 15995; previous integration is from x, y = 8.028, 2079 to 8.063, 3068 and previous response = 14967.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 12:26:27 PM	Zero out primary peak of compound Acenaphthene in sample Jan1045.D			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/11/2022 12:26:38 PM	Manually integrate qualifier 167.0 of compound Fluorene in sample Jan1045.D, from x, y = 8.674, 603 to 8.711, 716, result = 4581; previous integration is from x, y = 8.648, 676 to 8.773, 676 and previous response = 11590.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/11/2022 12:26:44 PM	Manually integrate qualifier 167.0 of compound Fluorene in sample Jan1045.D, from x, y = 8.686, 642 to 8.711, 716, result = 3131; previous integration is from x, y = 8.674, 603 to 8.711, 716 and previous response = 4581.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 12:26:46 PM	Drop baseline for qualifier 167.0 of compound Fluorene in sample Jan1045.D to y = 642, new integration is from x, y = 8.686, 642 to 8.711, 642 and new response = 3187; previous integration is from x, y = 8.686, 642 to 8.711, 716 and previous response = 3131.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 12:26:56 PM	Zero out primary peak of compound Acenaphthylene in sample Jan1045.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 12:27:03 PM	Manually integrate compound Benzo(a)pyrene in sample Jan1045.D, from x, y = 18.376, 43 to 18.450, 65, result = 161; previous integration is from x, y = 18.475, 67 to 18.660, 69 and previous response = 2275.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/11/2022 12:27:04 PM	Snap baseline for compound Benzo(a)pyrene in sample Jan1045.D, from x = 18.376 to x = 18.450, new integration is from x, y = 18.376, 65 to 18.450, 65 and new response = 113; previous integration is from x, y = 18.376, 43 to 18.450, 65 and previous response = 161.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 12:27:04 PM	Drop baseline for compound Benzo(a)pyrene in sample Jan1045.D to y = 65, new integration is from x, y = 18.376, 65 to 18.450, 65 and new response = 113; previous integration is from x, y = 18.376, 65 to 18.450, 65 and previous response = 113.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdZeroOutPeak	BL2000\jheine	1/11/2022 12:27:12 PM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1045.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/11/2022 12:27:19 PM	Manually integrate compound Chrysene in sample Jan1045.D, from x, y = 14.789, 237 to 14.863, 197, result = -262; previous integration is from x, y = 14.678, 57 to 14.789, 60 and previous response = 2248.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/11/2022 12:27:20 PM	Snap baseline for compound Chrysene in sample Jan1045.D, from x = 14.789 to x = 14.863, new integration is from x, y = 14.789, 152 to 14.863, 80 and new response = 192; previous integration is from x, y = 14.789, 237 to 14.863, 197 and previous response = -262.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 12:27:21 PM	Drop baseline for compound Chrysene in sample Jan1045.D to y = 80, new integration is from x, y = 14.789, 80 to 14.863, 80 and new response = 353; previous integration is from x, y = 14.789, 152 to 14.863, 80 and previous response = 192.			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 12:27:23 PM	Zero out primary peak of compound Chrysene in sample Jan1045.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 12:27:27 PM	Zero out primary peak of compound Anthracene in sample Jan1045.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 12:27:28 PM	Zero out primary peak of compound Phenanthrene in sample Jan1045.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/11/2022 12:27:29 PM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1045.D			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/11/2022 12:27:50 PM	Manually integrate qualifier 167.0 of compound Fluorene in sample Jan1045.D, from x, y = 8.636, 636 to 8.686, 748, result = 2502; previous integration is from x, y = 8.686, 642 to 8.711, 642 and previous response = 3187.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/11/2022 12:28:03 PM	Snap baseline for qualifier 167.0 of compound Fluorene in sample Jan1045.D from x = 8.636 to x = 8.686, new integration is from x, y = 8.636, 559 to 8.686, 2403 and new response = 142; previous integration is from x, y = 8.636, 636 to 8.686, 748 and previous response = 2502.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/11/2022 12:28:04 PM	Drop baseline for qualifier 167.0 of compound Fluorene in sample Jan1045.D to y = 559, new integration is from x, y = 8.636, 559 to 8.686, 559 and new response = 2900; previous integration is from x, y = 8.636, 559 to 8.686, 2403 and previous response = 142.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSaveBatchTable	BL2000\jheine	1/11/2022 12:28:23 PM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\2 e8270d bna SIM\QuantResults\011022 bna SIM 2.batch.bin			✓	
CmdSaveBatchTable	BL2000\jheine	1/11/2022 12:28:59 PM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\2 e8270d bna SIM\QuantResults\011022 bna SIM 2.batch.bin			✓	
CmdOpenBatchTable	BL2000\jheine	1/12/2022 8:25:24 AM	Open batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\2 e8270d bna SIM\011022 bna SIM 2.batch.bin			✓	
CmdSetSampleAttribute	BL2000\jheine	1/12/2022 8:26:03 AM	Set SampleApproved = True for sample Jan1041.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/12/2022 8:26:04 AM	Set SampleApproved = True for sample Jan1042.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/12/2022 8:26:05 AM	Set SampleApproved = True for sample Jan1043.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/12/2022 8:26:06 AM	Set SampleApproved = True for sample Jan1044.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/12/2022 8:26:07 AM	Set SampleApproved = True for sample Jan1045.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/12/2022 8:26:09 AM	Set SampleApproved = True for sample Jan1046.D; previous value = False			✓	
CmdZeroOutPeak	BL2000\jheine	1/12/2022 8:30:41 AM	Zero out primary peak of compound Fluorene in sample Jan1045.D			✓	
CmdSaveBatchTable	BL2000\jheine	1/12/2022 8:31:12 AM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\2 e8270d bna SIM\QuantResults\011022 bna SIM 2.batch.bin			✓	
CmdOpenBatchTable	BL2000\jheine	1/19/2022 5:37:39 PM	Open batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\2 e8270d bna SIM\011022 bna SIM 2.batch.bin			✓	
CmdQuantitate	BL2000\jheine	1/19/2022 5:47:01 PM	Quantitate all compounds in all samples			✓	
CmdSaveBatchTable	BL2000\jheine	1/19/2022 5:47:07 PM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011022\2 e8270d bna SIM\QuantResults\011022 bna SIM 2.batch.bin			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
GenerateReport	BL2000\jheine	1/19/2022 5:55:26 PM	Generates report - Method: D:\Org\reports\GCMSEMI Report Templates\Tests_for_LevelIV\Env_QuantResults_wGraphics+Chromatogram.m, Output Path: \\MASSHUNTER\Org\Data\SV5975.I\sh011022\2 e8270d bna SIM\QuantReports\			✓	

PREP BATCH REPORT

Prep Code: **SVOC-3510C-8270**
 Prep Batch **162744** Prep Temp **NA °C**

Technician: **Zachary B. Zaccardi**
 Batch Units: **ML**

Prep Start Date: **1/6/2022 9:18:55 AM**
 Prep End Date: **1/7/2022 4:25:00 PM**

Sample ID	Matrix	pH	Initial Samp Amt	Sol Added	Sol Recovered	Final Vol (mL)	Factor	Balance	Prep Start Date	Prep End Date
MB-162744			1000	0	0	1.00	0.001		1/6/2022	1/7/2022
	Supervised by RJB									
LCS-162744			1000	0	0	1.00	0.001		1/6/2022	1/7/2022
LCSD-162744			1000	0	0	1.00	0.001		1/6/2022	1/7/2022
B22010213-001C	Ground Water	6	970	0	0	1.00	0.00103		1/6/2022	1/7/2022
	Sample was clear (1/2)									
B22010213-002A	Ground Water	6	1010	0	0	1.00	0.00099		1/6/2022	1/7/2022
	Sample was clear (1/2)									
B22010213-003C	Ground Water	6	970	0	0	1.00	0.00103		1/6/2022	1/7/2022
	Sample was clear (1/2)									
B22010214-001C	Ground Water	6	970	0	0	1.00	0.00103		1/6/2022	1/7/2022
	Sample was clear (1/2)									
B22010219-001C	Drinking Water	6	970	0	0	1.00	0.00103		1/6/2022	1/7/2022
	Sample was clear (1/2)									
B22010227-002E	Aqueous	6	990	0	0	1.00	0.00101		1/6/2022	1/7/2022
	Sample was a cloudy yellow									
B22010249-002E	Aqueous	6	1050	0	0	1.00	0.000952		1/6/2022	1/7/2022
	Sample was cloudy with green organic material present									
B22010255-001B	Aqueous	6	1050	0	0	1.00	0.000952		1/6/2022	1/7/2022
	Sample was clear									
B22010213-001CMS	Ground Water	6	1030	0	0	1.00	0.000971		1/6/2022	1/7/2022
	Sample was clear (2/2)									
B22010213-002AMS	Ground Water	6	1030	0	0	1.00	0.000971		1/6/2022	1/7/2022
	Sample was clear (2/2)									
B22010213-003CLMS	Ground Water	6	1010	0	0	1.00	0.00099		1/6/2022	1/7/2022
	Sample was clear (2/2)									
LLCS-162744			1000	0	0	1.00	0.001		1/6/2022	1/7/2022

Number	Reagent Name	Exp Date	
13124	Sulfuric Acid 2020070739	7/2/2022	2mL
13273	pH-indicator Strips 0-14 HC025486	9/30/2024	
14196	Dichloromethane EB867	6/18/2023	100.50
14647	Dichloromethane EC832	10/28/2023	

Spk ID	Spike Name	SampType	AmtAdd	Exp Date
FP211227 14446	DCM RINSED FILTER PAPER	ALL		4/6/2026
Sulfate 12/27/21	Baked Sodium Sulfate	ALL	varies	11/29/2026
sv92616	APPIIA/Acetone	APP2A/D	1.0 mL	9/24/2022
sv83418	Benzidines	LCS, MS	50 uL	3/17/2024
sv92710	LCS/Add Extractions	LCS, MS; LLCS/D	1.0 mL; 5	1/14/2022
SVOC NaOH 122	10 N NaOH	MB, LCS, SAMP,	5 drops	7/31/2023
sv92712	LL BNA Surr	SAMP, LMS, LLC	100 uL	1/30/2022
sv92706	BNA Surr	SAMP, MB, LCS,	100 uL	3/31/2022

PREP BATCH REPORT

Prep Code: **SVOC-3510C-8270**
 Prep Batch **162744** Prep Temp **NA °C**

Technician: **Zachary B. Zaccardi**
 Batch Units: **ML**

Prep Start Date: **1/6/2022 9:18:55 AM**
 Prep End Date: **1/7/2022 4:25:00 PM**

Sample ID	Matrix	pH	Initial Samp Amt	Sol Added	Sol Recovered	Final Vol (mL)	Factor	Balance	Prep Start Date	Prep End Date
LLCSD-162744			1000	0	0	1.00	0.001		1/6/2022	1/7/2022
APP2A-162744			1000	0	0	1.00	0.001		1/6/2022	1/7/2022
APP2AD-162744			1000	0	0	1.00	0.001		1/6/2022	1/7/2022

Number	Reagent Name	Exp Date	
13124	Sulfuric Acid 2020070739	7/2/2022	2mL
13273	pH-indicator Strips 0-14 HC025486	9/30/2024	
14196	Dichloromethane EB867	6/18/2023	100,50
14647	Dichloromethane EC832	10/28/2023	

Spk ID	Spike Name	SampType	AmtAdd	Exp Date
FP211227 14446	DCM RINSED FILTER PAPER	ALL		4/6/2026
Sulfate 12/27/21 (Baked Sodium Sulfate	ALL	varies	11/29/2026
sv92616	APPIIA/Acetone	APP2A/D	1.0 mL	9/24/2022
sv83418	Benzidines	LCS, MS	50 uL	3/17/2024
sv92710	LCS/Add Extractions	LCS, MS; LLCSD	1.0 mL; 5	1/14/2022
SVOC NaOH 122	10 N NaOH	MB, LCS, SAMP,	5 drops	7/31/2023
sv92712	LL BNA Surr	SAMP, LMS, LLC	100 uL	1/30/2022
sv92706	BNA Surr	SAMP, MB, LCS,	100 uL	3/31/2022

Energy Laboratories Inc

ANALYTICAL RUN Summary

24-Feb-22

Run ID SV5975.I_220113A

Run Start Date: 1/13/2022
Analyst: John P. Heine
Ical:
Column ID: ZB-SemiVolatiles
Comments:

Std ID	Std Name	Std Amount	Std Units	Samp Amount	Samp Units	SampType	Expiration Date
dcmsvoc13	DCM						11/17/2022
sv100210	BNA 2nd source 200ug/mL	2	ul	198	ul	ICV	1/15/2022
sv100506	BNA low 50 ug/mL	8	ul	192	ul	CCV	3/31/2022
sv100703	BNA Internals 2000 ug/mL	2	ul	100	ul	SAMP	5/31/2022
sv83311	DFTPP 1000 ug/mL	50	ul	50	ul	TUNE	10/31/2022

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977426	Jan1301_D_TU	SVOC-8270-DF	TUNE	√5975.I\sh0113221	1/13/2022 3:19:0	1	R373164		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
127, % of mass 198	A	%	58.2	58.2		100	0	0	0	0.01	0	58%	40	60	0%	
197, % of mass 198	A	%	0	0		100	0	0	0	0.01	0	0%	0	0.99	0%	
198, Base Peak	A	%	100	100		100	0	0	0	0.01	0	100%	100	100	0%	
199, % of mass 198	A	%	7.2	7.2		100	0	0	0	0.01	0	7%	5	9	0%	
275, % of mass 198	A	%	26.5	26.5		100	0	0	0	0.01	0	27%	10	30	0%	
365, % of mass 198	A	%	2.5	2.5		100	0	0	0	0.01	0	3%	1	99.99	0%	
441, % of mass 443	A	%	92.6	92.6		100	0	0	0	0.01	0	93%	0.01	150	0%	
442, % of mass 198	A	%	57.9	57.9		100	0	0	0	0.01	0	58%	40	100	0%	
443, % of mass 442	A	%	19.1	19.1		100	0	0	0	0.01	0	19%	17	23	0%	
51, % of mass 198	A	%	52.6	52.6		100	0	0	0	0.01	0	53%	30	60	0%	
68, % of mass 69	A	%	0	0		100	0	0	0	0.01	0	0%	0	1.99	0%	
70, % of mass 69	A	%	0.6	0.6		100	0	0	0	0.01	0	1%	0	1.99	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977428	13-Jan-22_CCV	SVOC-8270-S-L	CCV	√5975.I\sh0113221	13/2022 3:43:2	1	R373164		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	mg/kg	2.19022	0.07300003		0.0667	0	0	0.000959	0.00333	10	109%	80	120	0%	
2-Methylnaphthalene	A	mg/kg	1.9352	0.06450022		0.0667	0	0	0.00088	0.00333	10	97%	80	120	0%	
Acenaphthene	A	mg/kg	1.98421	0.06613372		0.0667	0	0	0.000953	0.00333	10	99%	80	120	0%	
Acenaphthylene	A	mg/kg	2.21628	0.07386861		0.0667	0	0	0.000701	0.00333	10	111%	80	120	0%	
Anthracene	A	mg/kg	2.09278	0.06975236		0.0667	0	0	0.00141	0.00333	10	105%	80	120	0%	
Benzo(a)anthracene	A	mg/kg	2.1014	0.07003966		0.0667	0	0	0.00163	0.00333	10	105%	80	120	0%	
Benzo(a)pyrene	A	mg/kg	2.00586	0.06685531		0.0667	0	0	0.00135	0.00333	10	100%	80	120	0%	
Benzo(b)fluoranthene	A	mg/kg	1.80477	0.06015298		0.0667	0	0	0.00113	0.00333	10	90%	80	120	0%	
Benzo(g,h,i)perylene	A	mg/kg	2.05946	0.06864180		0.0667	0	0	0.00159	0.00333	10	103%	80	120	0%	
Benzo(k)fluoranthene	A	mg/kg	1.95827	0.06526914		0.0667	0	0	0.00153	0.00333	10	98%	80	120	0%	
Chrysene	A	mg/kg	2.10437	0.07013865		0.0667	0	0	0.00108	0.00333	10	105%	80	120	0%	
Dibenzo(a,h)anthracene	A	mg/kg	1.93848	0.06460954		0.0667	0	0	0.00143	0.00333	10	97%	80	120	0%	
Fluoranthene	A	mg/kg	1.83022	0.06100123		0.0667	0	0	0.00146	0.00333	10	91%	80	120	0%	
Fluorene	A	mg/kg	1.98423	0.06613439		0.0667	0	0	0.000856	0.00333	10	99%	80	120	0%	
Indeno(1,2,3-cd)pyrene	A	mg/kg	2.02604	0.06752791		0.0667	0	0	0.00189	0.00333	10	101%	80	120	0%	
Naphthalene	A	mg/kg	1.93186	0.06438889		0.0667	0	0	0.00104	0.00333	10	97%	80	120	0%	
Phenanthrene	A	mg/kg	1.99301	0.06642702		0.0667	0	0	0.00125	0.00333	10	100%	80	120	0%	
Pyrene	A	mg/kg	1.85417	0.06179949		0.0667	0	0	0.00155	0.00333	10	93%	80	120	0%	
1,4-Dichlorobenzene-d4	I	mg/kg	40	1.3332		0	0	0	0	0		0%	80	120	0%	
Acenaphthene-d10	I	mg/kg	40	1.3332		0	0	0	0	0		0%	80	120	0%	
Chrysene-d12	I	mg/kg	40	1.3332		0	0	0	0	0		0%	80	120	0%	
Naphthalene-d8	I	mg/kg	40	1.3332		0	0	0	0	0		0%	80	120	0%	
Perylene-d12	I	mg/kg	40	1.3332		0	0	0	0	0		0%	80	120	0%	
Phenanthrene-d10	I	mg/kg	40	1.3332		0	0	0	0	0		0%	80	120	0%	
2-Fluorobiphenyl	S	mg/kg	1.89936	0.06330567		0.0667	0	0	0.000818	0.00333	0	95%	80	120	0%	
Nitrobenzene-d5	S	mg/kg	1.69149	0.05637736		0.0667	0	0	0.00193	0.00333	0	85%	80	120	0%	
o-Terphenyl	S	mg/kg	1.65444	0.05514249		0.0667	0	0	0.00129	0.00333	150	83%	80	120	0%	
Terphenyl-d14	S	mg/kg	1.97141	0.0657071		0.0667	0	0	0.00154	0.00333	0	99%	80	120	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977429	13-Jan-22_ISTB	SVOC-8270-S-L	SAMP	√5975.I\sh0113221	13/2022 4:15:4	1	R373164		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977429	13-Jan-22_ISTB	SVOC-8270-S-L	SAMP	√5975.I\sh0113221	13/2022 4:15:4	1	R373164		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	mg/kg	0	0		0	0	0	0.000959	0.00333	10	0%	0	0	0%	
2-Methylnaphthalene	A	mg/kg	0	0		0	0	0	0.00088	0.00333	10	0%	0	0	0%	
Acenaphthene	A	mg/kg	0	0		0	0	0	0.000953	0.00333	10	0%	0	0	0%	
Acenaphthylene	A	mg/kg	0	0		0	0	0	0.000701	0.00333	10	0%	0	0	0%	
Anthracene	A	mg/kg	0	0		0	0	0	0.00141	0.00333	10	0%	0	0	0%	
Benzo(a)anthracene	A	mg/kg	0	0		0	0	0	0.00163	0.00333	10	0%	0	0	0%	
Benzo(a)pyrene	A	mg/kg	0	0		0	0	0	0.00135	0.00333	10	0%	0	0	0%	
Benzo(b)fluoranthene	A	mg/kg	0	0		0	0	0	0.00113	0.00333	10	0%	0	0	0%	
Benzo(g,h,i)perylene	A	mg/kg	0	0		0	0	0	0.00159	0.00333	10	0%	0	0	0%	
Benzo(k)fluoranthene	A	mg/kg	0	0		0	0	0	0.00153	0.00333	10	0%	0	0	0%	
Chrysene	A	mg/kg	0	0		0	0	0	0.00108	0.00333	10	0%	0	0	0%	
Dibenzo(a,h)anthracene	A	mg/kg	0	0		0	0	0	0.00143	0.00333	10	0%	0	0	0%	
Fluoranthene	A	mg/kg	0	0		0	0	0	0.00146	0.00333	10	0%	0	0	0%	
Fluorene	A	mg/kg	0	0		0	0	0	0.000856	0.00333	10	0%	0	0	0%	
Indeno(1,2,3-cd)pyrene	A	mg/kg	0	0		0	0	0	0.00189	0.00333	10	0%	0	0	0%	
Naphthalene	A	mg/kg	0	0		0	0	0	0.00104	0.00333	10	0%	0	0	0%	
Phenanthrene	A	mg/kg	0	0		0	0	0	0.00125	0.00333	10	0%	0	0	0%	
Pyrene	A	mg/kg	0	0		0	0	0	0.00155	0.00333	10	0%	0	0	0%	
1,4-Dichlorobenzene-d4	I	mg/kg	40	1.3332		0	0	0	0	0		0%	0	0	0%	
Acenaphthene-d10	I	mg/kg	40	1.3332		0	0	0	0	0		0%	0	0	0%	
Chrysene-d12	I	mg/kg	40	1.3332		0	0	0	0	0		0%	0	0	0%	
Naphthalene-d8	I	mg/kg	40	1.3332		0	0	0	0	0		0%	0	0	0%	
Perylene-d12	I	mg/kg	40	1.3332		0	0	0	0	0		0%	0	0	0%	
Phenanthrene-d10	I	mg/kg	40	1.3332		0	0	0	0	0		0%	0	0	0%	
2-Fluorobiphenyl	S	mg/kg	0	0		0.167	0	0	0.000818	0.00333	0	0%	47	110	0%	S
Nitrobenzene-d5	S	mg/kg	0	0		0.167	0	0	0.00193	0.00333	0	0%	43	105	0%	S
Terphenyl-d14	S	mg/kg	0	0		0.167	0	0	0.00154	0.00333	0	0%	51	117	0%	S
o-Terphenyl	X	mg/kg	0	0		6.67	0	0	0.00129	0.00333	150	0%	40	140	0%	S

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977430	B22010648-005	SVOC-8270-S-L	SAMP	√5975.I\sh0113221	13/2022 4:48:1	1	162835	12/22/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977430	B22010648-005	SVOC-8270-S-L	SAMP	√5975.I\sh0113221	13/2022 4:48:1	1	162835	12/22/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	mg/kg	0.22742	0.01736124		0	0	0	0.0021963	0.0076264	10	0%	0	0	0%	
2-Methylnaphthalene	A	mg/kg	0.26339	0.02010719		0	0	0	0.0020154	0.0076264	10	0%	0	0	0%	
Acenaphthene	A	mg/kg	0.28901	0.02206302		0	0	0	0.0021826	0.0076264	10	0%	0	0	0%	
Acenaphthylene	A	mg/kg	0	0		0	0	0	0.0016054	0.0076264	10	0%	0	0	0%	
Anthracene	A	mg/kg	0.83708	0.06390269		0	0	0	0.0032292	0.0076264	10	0%	0	0	0%	
Benzo(a)anthracene	A	mg/kg	1.6975	0.12958715		0	0	0	0.0037330	0.0076264	10	0%	0	0	0%	
Benzo(a)pyrene	A	mg/kg	1.62043	0.12370363		0	0	0	0.0030918	0.0076264	10	0%	0	0	0%	
Benzo(b)fluoranthene	A	mg/kg	1.45081	0.11075484		0	0	0	0.0025879	0.0076264	10	0%	0	0	0%	
Benzo(g,h,i)perylene	A	mg/kg	1.57421	0.12017519		0	0	0	0.0036414	0.0076264	10	0%	0	0	0%	
Benzo(k)fluoranthene	A	mg/kg	1.32161	0.10089171		0	0	0	0.0035040	0.0076264	10	0%	0	0	0%	
Chrysene	A	mg/kg	2.14315	0.16360807		0	0	0	0.0024734	0.0076264	10	0%	0	0	0%	
Dibenzo(a,h)anthracene	A	mg/kg	1.21106	0.09245232		0	0	0	0.003275	0.0076264	10	0%	0	0	0%	
Fluoranthene	A	mg/kg	1.40397	0.10717907		0	0	0	0.0033437	0.0076264	10	0%	0	0	0%	
Fluorene	A	mg/kg	0.4002	0.03055127		0	0	0	0.0019604	0.0076264	10	0%	0	0	0%	
Indeno(1,2,3-cd)pyrene	A	mg/kg	1.52573	0.11647423		0	0	0	0.0043285	0.0076264	10	0%	0	0	0%	
Naphthalene	A	mg/kg	0.42782	0.03265978		0	0	0	0.0023818	0.0076264	10	0%	0	0	0%	B
Phenanthrene	A	mg/kg	1.46778	0.11205033		0	0	0	0.0028628	0.0076264	10	0%	0	0	0%	
Pyrene	A	mg/kg	1.8199	0.13893117		0	0	0	0.0035498	0.0076264	10	0%	0	0	0%	
1,4-Dichlorobenzene-d4	I	mg/kg	40	3.0536		0	0	0	0	0		0%	0	0	0%	
Acenaphthene-d10	I	mg/kg	40	3.0536		0	0	0	0	0		0%	0	0	0%	
Chrysene-d12	I	mg/kg	40	3.0536		0	0	0	0	0		0%	0	0	0%	
Naphthalene-d8	I	mg/kg	40	3.0536		0	0	0	0	0		0%	0	0	0%	
Perylene-d12	I	mg/kg	40	3.0536		0	0	0	0	0		0%	0	0	0%	
Phenanthrene-d10	I	mg/kg	40	3.0536		0	0	0	0	0		0%	0	0	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977431	B22010648-005	SVOC-8270-S-L	SAMP	√5975.I\sh0113221	13/2022 5:20:4	20	162835	12/22/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
2-Fluorobiphenyl	S	mg/kg	3.92876	5.99843077		7.63715	0	0	0.0374677	0.1525273	0	79%	40	140	0%	
o-Terphenyl	S	mg/kg	3.43217	5.24023716		7.63715	0	0	0.0590872	0.1525273	150	69%	40	140	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977432	MB-162744	SVOC-8270C-SI	MBLK	√5975.I\sh0113221	13/2022 5:53:1	1	162744	1/6/2022 9:1	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0206	0.1	10	0%			0%	
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0176	0.1	10	0%			0%	
Acenaphthene	A	ug/L	0	0		0	0	0	0.0317	0.1	10	0%			0%	
Acenaphthylene	A	ug/L	0	0		0	0	0	0.025	0.1	10	0%			0%	
Anthracene	A	ug/L	0	0		0	0	0	0.0283	0.1	10	0%			0%	
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.0272	0.1	10	0%			0%	
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.0347	0.1	10	0%			0%	
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.0226	0.1	10	0%			0%	
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.0267	0.1	10	0%			0%	
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.0295	0.1	10	0%			0%	
Chrysene	A	ug/L	0	0		0	0	0	0.0458	0.1	10	0%			0%	
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.0367	0.1	10	0%			0%	
Fluoranthene	A	ug/L	0	0		0	0	0	0.0233	0.1	10	0%			0%	
Fluorene	A	ug/L	0	0		0	0	0	0.0225	0.1	10	0%			0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.0491	0.1	10	0%			0%	
Naphthalene	A	ug/L	0	0		0	0	0	0.029	0.1	10	0%			0%	
Phenanthrene	A	ug/L	0	0		0	0	0	0.0295	0.1	10	0%			0%	
Pyrene	A	ug/L	0	0		0	0	0	0.0239	0.1	10	0%			0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977433	LLCS-162744	SVOC-8270C-SI	LCS-DOD	√5975.I\sh0113221	13/2022 6:25:3	1	162744	1/6/2022 3:2	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	3.46546	3.46546		5	0	0	0.0206	0.1	10	69%	41	115	0%	
2-Methylnaphthalene	A	ug/L	3.51741	3.51741		5	0	0	0.0176	0.1	10	70%	39	114	0%	
Acenaphthene	A	ug/L	3.67134	3.67134		5	0	0	0.0317	0.1	10	73%	48	114	0%	
Acenaphthylene	A	ug/L	4.06287	4.06287		5	0	0	0.025	0.1	10	81%	35	121	0%	
Anthracene	A	ug/L	4.66776	4.66776		5	0	0	0.0283	0.1	10	93%	53	119	0%	
Benzo(a)anthracene	A	ug/L	4.90876	4.90876		5	0	0	0.0272	0.1	10	98%	59	120	0%	
Benzo(a)pyrene	A	ug/L	4.23483	4.23483		5	0	0	0.0347	0.1	10	85%	53	120	0%	
Benzo(b)fluoranthene	A	ug/L	3.998	3.998		5	0	0	0.0226	0.1	10	80%	53	126	0%	
Benzo(g,h,i)perylene	A	ug/L	4.57023	4.57023		5	0	0	0.0267	0.1	10	91%	44	128	0%	
Benzo(k)fluoranthene	A	ug/L	4.04615	4.04615		5	0	0	0.0295	0.1	10	81%	54	125	0%	
Chrysene	A	ug/L	4.59003	4.59003		5	0	0	0.0458	0.1	10	92%	57	120	0%	
Dibenzo(a,h)anthracene	A	ug/L	4.89796	4.89796		5	0	0	0.0367	0.1	10	98%	44	141	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977433	LLCS-162744	SVOC-8270C-SI	LCS-DOD	√5975.I\sh0113221	13/2022 6:25:3	1	162744	1/6/2022 3:2	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Fluoranthene	A	ug/L	4.02653	4.02653		5	0	0	0.0233	0.1	10	81%	58	120	0%	
Fluorene	A	ug/L	3.77721	3.77721		5	0	0	0.0225	0.1	10	76%	50	118	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	4.82805	4.82805		5	0	0	0.0491	0.1	10	97%	48	130	0%	
Naphthalene	A	ug/L	3.44089	3.44089		5	0	0	0.029	0.1	10	69%	43	114	0%	
Phenanthrene	A	ug/L	4.35875	4.35875		5	0	0	0.0295	0.1	10	87%	53	115	0%	
Pyrene	A	ug/L	4.19455	4.19455		5	0	0	0.0239	0.1	10	84%	53	121	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1	10	0%			0%	
2-Fluorobiphenyl	S	ug/L	3.29006	3.29006		5	0	0	0.0444	0.1	10	66%	53	106	0%	
Nitrobenzene-d5	S	ug/L	3.45504	3.45504		5	0	0	0.0523	0.1	10	69%	55	111	0%	
Terphenyl-d14	S	ug/L	4.54643	4.54643		5	0	0	0.0563	0.1	10	91%	58	132	0%	
o-Terphenyl	X	ug/L	3.20913	3.20913		5	0	0	0.0654	0	0	64%	40	140	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977434	LLCSD-162744	SVOC-8270C-SI	LCSD-DOD	√5975.I\sh0113221	13/2022 6:58:0	1	162744	1/6/2022 3:2	0	1E+07						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	2.8637	2.8637		5	0	3.46546	0.0206	0.1	10	57%	41	115	19%	
2-Methylnaphthalene	A	ug/L	3.01152	3.01152		5	0	3.51741	0.0176	0.1	10	60%	39	114	15%	
Acenaphthene	A	ug/L	3.79592	3.79592		5	0	3.67134	0.0317	0.1	10	76%	48	114	3%	
Acenaphthylene	A	ug/L	4.05711	4.05711		5	0	4.06287	0.025	0.1	10	81%	35	121	0%	
Anthracene	A	ug/L	4.78934	4.78934		5	0	4.66776	0.0283	0.1	10	96%	53	119	3%	
Benzo(a)anthracene	A	ug/L	5.08735	5.08735		5	0	4.90876	0.0272	0.1	10	102%	59	120	4%	
Benzo(a)pyrene	A	ug/L	4.33705	4.33705		5	0	4.23483	0.0347	0.1	10	87%	53	120	2%	
Benzo(b)fluoranthene	A	ug/L	4.22003	4.22003		5	0	3.998	0.0226	0.1	10	84%	53	126	5%	
Benzo(g,h,i)perylene	A	ug/L	4.68845	4.68845		5	0	4.57023	0.0267	0.1	10	94%	44	128	3%	
Benzo(k)fluoranthene	A	ug/L	4.20937	4.20937		5	0	4.04615	0.0295	0.1	10	84%	54	125	4%	
Chrysene	A	ug/L	4.75365	4.75365		5	0	4.59003	0.0458	0.1	10	95%	57	120	4%	
Dibenzo(a,h)anthracene	A	ug/L	4.69063	4.69063		5	0	4.89796	0.0367	0.1	10	94%	44	141	4%	
Fluoranthene	A	ug/L	4.26574	4.26574		5	0	4.02653	0.0233	0.1	10	85%	58	120	6%	
Fluorene	A	ug/L	3.90488	3.90488		5	0	3.77721	0.0225	0.1	10	78%	50	118	3%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977434	LLCSD-162744	SVOC-8270C-SI	LCSD-DOD	√5975.I\sh0113221	13/2022 6:58:0	1	162744	1/6/2022 3:2	0	1E+07						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Indeno(1,2,3-cd)pyrene	A	ug/L	4.87241	4.87241		5	0	4.82805	0.0491	0.1	10	97%	48	130	1%	
Naphthalene	A	ug/L	2.96644	2.96644		5	0	3.44089	0.029	0.1	10	59%	43	114	15%	
Phenanthrene	A	ug/L	4.4789	4.4789		5	0	4.35875	0.0295	0.1	10	90%	53	115	3%	
Pyrene	A	ug/L	4.38756	4.38756		5	0	4.19455	0.0239	0.1	10	88%	53	121	4%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%				0%
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%				0%
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%				0%
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%				0%
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%				0%
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1	10	0%				0%
2-Fluorobiphenyl	S	ug/L	3.14547	3.14547		5	0	0	0.0444	0.1	10	63%	53	106	0%	
Nitrobenzene-d5	S	ug/L	3.34068	3.34068		5	0	0	0.0523	0.1	10	67%	55	111	0%	
Terphenyl-d14	S	ug/L	4.68188	4.68188		5	0	0	0.0563	0.1	10	94%	58	132	0%	
o-Terphenyl	X	ug/L	3.51466	3.51466		5	0	3.20913	0.0654	0	0	70%	40	140	9%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977435	B22010213-001	SVOC-8270C-SI	SAMP	√5975.I\sh0113221	13/2022 7:30:3	1	162744	1/6/2022 9:1	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.021218	0.103	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.018128	0.103	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.032651	0.103	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.02575	0.103	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.029149	0.103	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.028016	0.103	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.035741	0.103	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.023278	0.103	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.027501	0.103	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.030385	0.103	10	0%	0	0	0%	U
Chrysene	A	ug/L	0	0		0	0	0	0.047174	0.103	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.037801	0.103	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0	0		0	0	0	0.023999	0.103	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.023175	0.103	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.050573	0.103	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.02987	0.103	10	0%	0	0	0%	U

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977435	B22010213-001	SVOC-8270C-SI SAMP		√5975.I\sh0113221	1/13/2022 7:30:3	1	162744	1/6/2022 9:1	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Phenanthrene	A	ug/L	0	0		0	0	0	0.030385	0.103	10	0%	0	0	0%	U
Pyrene	A	ug/L	0	0		0	0	0	0.024617	0.103	10	0%	0	0	0%	U

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977436	B22010213-002	SVOC-8270C-SI SAMP		√5975.I\sh0113221	1/13/2022 8:03:0	1	162744	1/6/2022 9:1	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.020394	0.1	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.017424	0.1	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.031383	0.1	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.02475	0.1	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.028017	0.1	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.026928	0.1	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.034353	0.1	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.022374	0.1	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.026433	0.1	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.029205	0.1	10	0%	0	0	0%	U
Chrysene	A	ug/L	0	0		0	0	0	0.045342	0.1	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.036333	0.1	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0	0		0	0	0	0.023067	0.1	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.022275	0.1	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.048609	0.1	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.02871	0.1	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.029205	0.1	10	0%	0	0	0%	U
Pyrene	A	ug/L	0	0		0	0	0	0.023661	0.1	10	0%	0	0	0%	U

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977437	B22010213-003	SVOC-8270C-SI SAMP		√5975.I\sh0113221	1/13/2022 8:35:1	1	162744	1/6/2022 9:1	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.021218	0.103	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.018128	0.103	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.032651	0.103	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.02575	0.103	10	0%	0	0	0%	U

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977437	B22010213-003	SVOC-8270C-SI SAMP		√5975.I\sh0113221	13/2022 8:35:1	1	162744	1/6/2022 9:1	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Anthracene	A	ug/L	0	0		0	0	0	0.029149	0.103	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.028016	0.103	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.035741	0.103	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.023278	0.103	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.027501	0.103	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.030385	0.103	10	0%	0	0	0%	U
Chrysene	A	ug/L	0	0		0	0	0	0.047174	0.103	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.037801	0.103	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0	0		0	0	0	0.023999	0.103	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.023175	0.103	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.050573	0.103	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.02987	0.103	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.030385	0.103	10	0%	0	0	0%	U
Pyrene	A	ug/L	0	0		0	0	0	0.024617	0.103	10	0%	0	0	0%	U

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977438	B22010213-003	SVOC-8270C-SI MS-DOD		√5975.I\sh0113221	13/2022 9:08:0	1	162744	1/6/2022 1:0	1E+07	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	2.93271	2.9033829		4.95	0	0	0.020394	0.1	10	59%	41	115	0%	
2-Methylnaphthalene	A	ug/L	2.85169	2.8231731		4.95	0	0	0.017424	0.1	10	57%	39	114	0%	
Acenaphthene	A	ug/L	3.20107	3.1690593		4.95	0	0	0.031383	0.1	10	64%	48	114	0%	
Acenaphthylene	A	ug/L	3.81329	3.7751571		4.95	0	0	0.02475	0.1	10	76%	35	121	0%	
Anthracene	A	ug/L	4.50343	4.4583957		4.95	0	0	0.028017	0.1	10	90%	53	119	0%	
Benzo(a)anthracene	A	ug/L	4.95274	4.9032126		4.95	0	0	0.026928	0.1	10	99%	59	120	0%	
Benzo(a)pyrene	A	ug/L	3.96522	3.9255678		4.95	0	0	0.034353	0.1	10	79%	53	120	0%	
Benzo(b)fluoranthene	A	ug/L	3.87429	3.8355471		4.95	0	0	0.022374	0.1	10	77%	53	126	0%	
Benzo(g,h,i)perylene	A	ug/L	4.05506	4.0145094		4.95	0	0	0.026433	0.1	10	81%	44	128	0%	
Benzo(k)fluoranthene	A	ug/L	3.69301	3.6560799		4.95	0	0	0.029205	0.1	10	74%	54	125	0%	
Chrysene	A	ug/L	4.4683	4.423617		4.95	0	0	0.045342	0.1	10	89%	57	120	0%	
Dibenzo(a,h)anthracene	A	ug/L	4.28447	4.2416253		4.95	0	0	0.036333	0.1	10	86%	44	141	0%	
Fluoranthene	A	ug/L	4.06003	4.0194297		4.95	0	0	0.023067	0.1	10	81%	58	120	0%	
Fluorene	A	ug/L	3.49495	3.4600005		4.95	0	0	0.022275	0.1	10	70%	50	118	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	4.34236	4.2989364		4.95	0	0	0.048609	0.1	10	87%	48	130	0%	
Naphthalene	A	ug/L	2.90843	2.8793457		4.95	0	0	0.02871	0.1	10	58%	43	114	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977438	B22010213-003	SVOC-8270C-SI	MS-DOD	√5975.I\sh0113221	13/2022 9:08:0	1	162744	1/6/2022 1:0	1E+07	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Phenanthrene	A	ug/L	3.508	3.47292		4.95	0	0	0.029205	0.1	10	70%	53	115	0%	
Pyrene	A	ug/L	4.13236	4.0910364		4.95	0	0	0.023661	0.1	10	83%	53	121	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	39.6		0	0	0	0.099	0.1		0%			0%	
Acenaphthene-d10	I	ug/L	40	39.6		0	0	0	0.099	0.1		0%			0%	
Chrysene-d12	I	ug/L	40	39.6		0	0	0	0.099	0.1		0%			0%	
Naphthalene-d8	I	ug/L	40	39.6		0	0	0	0.099	0.1		0%			0%	
Perylene-d12	I	ug/L	40	39.6		0	0	0	0.099	0.1		0%			0%	
Phenanthrene-d10	I	ug/L	40	39.6		0	0	0	0.099	0.1	10	0%			0%	
2-Fluorobiphenyl	S	ug/L	3.24292	3.2104908		4.95	0	0	0.043956	0.1	10	65%	53	106	0%	
Nitrobenzene-d5	S	ug/L	3.64968	3.6131832		4.95	0	0	0.051777	0.1	10	73%	55	111	0%	
Terphenyl-d14	S	ug/L	4.388	4.34412		4.95	0	0	0.055737	0.1	10	88%	58	132	0%	
o-Terphenyl	X	ug/L	3.32107	3.2878593		4.95	0	0	0.064746	0	0	66%	40	140	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977439	B22010214-001	SVOC-8270C-SI	SAMP	√5975.I\sh0113221	13/2022 9:40:2	1	162744	1/6/2022 9:1	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.021218	0.103	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.018128	0.103	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.032651	0.103	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.02575	0.103	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.029149	0.103	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.028016	0.103	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.035741	0.103	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.023278	0.103	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.027501	0.103	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.030385	0.103	10	0%	0	0	0%	U
Chrysene	A	ug/L	0	0		0	0	0	0.047174	0.103	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.037801	0.103	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0	0		0	0	0	0.023999	0.103	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.023175	0.103	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.050573	0.103	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.02987	0.103	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.030385	0.103	10	0%	0	0	0%	U
Pyrene	A	ug/L	0	0		0	0	0	0.024617	0.103	10	0%	0	0	0%	U

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977439	B22010214-001	SVOC-8270C-SI SAMP		√5975.I\sh0113221	13/2022 9:40:2	1	162744	1/6/2022 9:1	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977440	B22010219-001	SVOC-8270C-SI SAMP		√5975.I\sh0113221	13/2022 10:12:	1	162744	1/6/2022 9:1	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.021218	0.103	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.018128	0.103	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.032651	0.103	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.02575	0.103	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.029149	0.103	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.028016	0.103	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.035741	0.103	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.023278	0.103	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.027501	0.103	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.030385	0.103	10	0%	0	0	0%	U
Chrysene	A	ug/L	0	0		0	0	0	0.047174	0.103	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.037801	0.103	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0	0		0	0	0	0.023999	0.103	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.023175	0.103	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.050573	0.103	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.02987	0.103	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.030385	0.103	10	0%	0	0	0%	U
Pyrene	A	ug/L	0	0		0	0	0	0.024617	0.103	10	0%	0	0	0%	U

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977468	13-Jan-22_CC	SVOC-8270C-SI CCV		√5975.I\sh0113221	13/2022 3:43:2	1	R373164		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

1-Methylnaphthalene	A	ug/L	2.19022	2.19022		2	0	0	0.0206	0.1	10	110%	80	120	0%	
2-Methylnaphthalene	A	ug/L	1.9352	1.9352		2	0	0	0.0176	0.1	10	97%	80	120	0%	
Acenaphthene	A	ug/L	1.98421	1.98421		2	0	0	0.0317	0.1	10	99%	80	120	0%	
Acenaphthylene	A	ug/L	2.21628	2.21628		2	0	0	0.025	0.1	10	111%	80	120	0%	
Anthracene	A	ug/L	2.09278	2.09278		2	0	0	0.0283	0.1	10	105%	80	120	0%	
Benzo(a)anthracene	A	ug/L	2.1014	2.1014		2	0	0	0.0272	0.1	10	105%	80	120	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977468	13-Jan-22_CCV	SVOC-8270C-SI	CCV	√5975.I\sh0113221	13/2022 3:43:2	1	R373164		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Benzo(a)pyrene	A	ug/L	2.00586	2.00586		2	0	0	0.0347	0.1	10	100%	80	120	0%	
Benzo(b)fluoranthene	A	ug/L	1.80477	1.80477		2	0	0	0.0226	0.1	10	90%	80	120	0%	
Benzo(g,h,i)perylene	A	ug/L	2.05946	2.05946		2	0	0	0.0267	0.1	10	103%	80	120	0%	
Benzo(k)fluoranthene	A	ug/L	1.95827	1.95827		2	0	0	0.0295	0.1	10	98%	80	120	0%	
Chrysene	A	ug/L	2.10437	2.10437		2	0	0	0.0458	0.1	10	105%	80	120	0%	
Dibenzo(a,h)anthracene	A	ug/L	1.93848	1.93848		2	0	0	0.0367	0.1	10	97%	80	120	0%	
Fluoranthene	A	ug/L	1.83022	1.83022		2	0	0	0.0233	0.1	10	92%	80	120	0%	
Fluorene	A	ug/L	1.98423	1.98423		2	0	0	0.0225	0.1	10	99%	80	120	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	2.02604	2.02604		2	0	0	0.0491	0.1	10	101%	80	120	0%	
Naphthalene	A	ug/L	1.93186	1.93186		2	0	0	0.029	0.1	10	97%	80	120	0%	
Phenanthrene	A	ug/L	1.99301	1.99301		2	0	0	0.0295	0.1	10	100%	80	120	0%	
Pyrene	A	ug/L	1.85417	1.85417		2	0	0	0.0239	0.1	10	93%	80	120	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1	10	0%	80	120	0%	
2-Fluorobiphenyl	S	ug/L	1.89936	1.89936		2	0	0	0.0444	0.1	10	95%	80	120	0%	
Nitrobenzene-d5	S	ug/L	1.69149	1.69149		2	0	0	0.0523	0.1	10	85%	80	120	0%	
Terphenyl-d14	S	ug/L	1.97141	1.97141		2	0	0	0.0563	0.1	10	99%	80	120	0%	
o-Terphenyl	X	ug/L	1.65444	1.65444		2	0	0	0.0654	0	0	83%	80	120	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977469	13-Jan-22_CCV	SVOC-8270C-SI	CCV	√5975.I\sh0113221	13/2022 10:45:	1	R373164		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	2.30999	2.30999		2	0	0	0.0206	0.1	10	115%	50	150	0%	
2-Methylnaphthalene	A	ug/L	2.12763	2.12763		2	0	0	0.0176	0.1	10	106%	50	150	0%	
Acenaphthene	A	ug/L	2.11106	2.11106		2	0	0	0.0317	0.1	10	106%	50	150	0%	
Acenaphthylene	A	ug/L	2.34965	2.34965		2	0	0	0.025	0.1	10	117%	50	150	0%	
Anthracene	A	ug/L	2.31833	2.31833		2	0	0	0.0283	0.1	10	116%	50	150	0%	
Benzo(a)anthracene	A	ug/L	2.34071	2.34071		2	0	0	0.0272	0.1	10	117%	50	150	0%	
Benzo(a)pyrene	A	ug/L	2.05196	2.05196		2	0	0	0.0347	0.1	10	103%	50	150	0%	
Benzo(b)fluoranthene	A	ug/L	1.824	1.824		2	0	0	0.0226	0.1	10	91%	50	150	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977469	13-Jan-22_CCV	SVOC-8270C-SI CCV		√5975.I\sh0113221	13/2022 10:45:	1	R373164		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Benzo(g,h,i)perylene	A	ug/L	2.12396	2.12396		2	0	0	0.0267	0.1	10	106%	50	150	0%	
Benzo(k)fluoranthene	A	ug/L	1.87327	1.87327		2	0	0	0.0295	0.1	10	94%	50	150	0%	
Chrysene	A	ug/L	2.31362	2.31362		2	0	0	0.0458	0.1	10	116%	50	150	0%	
Dibenzo(a,h)anthracene	A	ug/L	1.95825	1.95825		2	0	0	0.0367	0.1	10	98%	50	150	0%	
Fluoranthene	A	ug/L	1.95923	1.95923		2	0	0	0.0233	0.1	10	98%	50	150	0%	
Fluorene	A	ug/L	2.18504	2.18504		2	0	0	0.0225	0.1	10	109%	50	150	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	2.07368	2.07368		2	0	0	0.0491	0.1	10	104%	50	150	0%	
Naphthalene	A	ug/L	2.20115	2.20115		2	0	0	0.029	0.1	10	110%	50	150	0%	
Phenanthrene	A	ug/L	2.10326	2.10326		2	0	0	0.0295	0.1	10	105%	50	150	0%	
Pyrene	A	ug/L	2.12725	2.12725		2	0	0	0.0239	0.1	10	106%	50	150	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%	50	150	0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%	50	150	0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	50	150	0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%	50	150	0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	50	150	0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1	10	0%	50	150	0%	
2-Fluorobiphenyl	S	ug/L	2.11001	2.11001		2	0	0	0.0444	0.1	10	106%	50	150	0%	
Nitrobenzene-d5	S	ug/L	2.02675	2.02675		2	0	0	0.0523	0.1	10	101%	50	150	0%	
Terphenyl-d14	S	ug/L	2.22004	2.22004		2	0	0	0.0563	0.1	10	111%	50	150	0%	
o-Terphenyl	X	ug/L	1.74729	1.74729		2	0	0	0.0654	0	0	87%	50	150	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15044402	LLCS-162744	SVOC-8270C-SI LCS		√5975.I\sh0113221	13/2022 6:25:3	1	162744	1/6/2022 3:2	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	3.46546	3.46546		5	0	0	0.0206	0.1	10	69%	18	117	0%	
2-Methylnaphthalene	A	ug/L	3.51741	3.51741		5	0	0	0.0176	0.1	10	70%	18	117	0%	
Acenaphthene	A	ug/L	3.67134	3.67134		5	0	0	0.0317	0.1	10	73%	40	92	0%	
Acenaphthylene	A	ug/L	4.06287	4.06287		5	0	0	0.025	0.1	10	81%	37	96	0%	
Anthracene	A	ug/L	4.66776	4.66776		5	0	0	0.0283	0.1	10	93%	46	108	0%	
Benzo(a)anthracene	A	ug/L	4.90876	4.90876		5	0	0	0.0272	0.1	10	98%	41	105	0%	
Benzo(a)pyrene	A	ug/L	4.23483	4.23483		5	0	0	0.0347	0.1	10	85%	42	110	0%	
Benzo(b)fluoranthene	A	ug/L	3.998	3.998		5	0	0	0.0226	0.1	10	80%	27	121	0%	
Benzo(g,h,i)perylene	A	ug/L	4.57023	4.57023		5	0	0	0.0267	0.1	10	91%	44	108	0%	
Benzo(k)fluoranthene	A	ug/L	4.04615	4.04615		5	0	0	0.0295	0.1	10	81%	44	111	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15044402	LLCS-162744	SVOC-8270C-SI LCS		√5975.I\sh0113221	13/2022 6:25:3	1	162744	1/6/2022 3:2	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Chrysene	A	ug/L	4.59003	4.59003		5	0	0	0.0458	0.1	10	92%	50	106	0%	
Dibenzo(a,h)anthracene	A	ug/L	4.89796	4.89796		5	0	0	0.0367	0.1	10	98%	47	111	0%	
Fluoranthene	A	ug/L	4.02653	4.02653		5	0	0	0.0233	0.1	10	81%	44	111	0%	
Fluorene	A	ug/L	3.77721	3.77721		5	0	0	0.0225	0.1	10	76%	42	99	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	4.82805	4.82805		5	0	0	0.0491	0.1	10	97%	33	112	0%	
Naphthalene	A	ug/L	3.44089	3.44089		5	0	0	0.029	0.1	10	69%	22	108	0%	
Phenanthrene	A	ug/L	4.35875	4.35875		5	0	0	0.0295	0.1	10	87%	43	106	0%	
Pyrene	A	ug/L	4.19455	4.19455		5	0	0	0.0239	0.1	10	84%	41	106	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1	10	0%			0%	
2-Fluorobiphenyl	S	ug/L	3.29006	3.29006		5	0	0	0.0444	0.1	10	66%	25	94	0%	
Nitrobenzene-d5	S	ug/L	3.45504	3.45504		5	0	0	0.0523	0.1	10	69%	19	102	0%	
Terphenyl-d14	S	ug/L	4.54643	4.54643		5	0	0	0.0563	0.1	10	91%	39	106	0%	
o-Terphenyl	X	ug/L	3.20913	3.20913		5	0	0	0.0654	0	0	64%	40	140	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15044403	LLCSD-162744	SVOC-8270C-SI LLCSD		√5975.I\sh0113221	13/2022 6:58:0	1	162744	1/6/2022 3:2	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	2.8637	2.8637		5	0	0	0.0206	0.1	10	57%	18	117	0%	
2-Methylnaphthalene	A	ug/L	3.01152	3.01152		5	0	0	0.0176	0.1	10	60%	18	117	0%	
Acenaphthene	A	ug/L	3.79592	3.79592		5	0	0	0.0317	0.1	10	76%	40	92	0%	
Acenaphthylene	A	ug/L	4.05711	4.05711		5	0	0	0.025	0.1	10	81%	37	96	0%	
Anthracene	A	ug/L	4.78934	4.78934		5	0	0	0.0283	0.1	10	96%	46	108	0%	
Benzo(a)anthracene	A	ug/L	5.08735	5.08735		5	0	0	0.0272	0.1	10	102%	41	105	0%	
Benzo(a)pyrene	A	ug/L	4.33705	4.33705		5	0	0	0.0347	0.1	10	87%	42	110	0%	
Benzo(b)fluoranthene	A	ug/L	4.22003	4.22003		5	0	0	0.0226	0.1	10	84%	27	121	0%	
Benzo(g,h,i)perylene	A	ug/L	4.68845	4.68845		5	0	0	0.0267	0.1	10	94%	44	108	0%	
Benzo(k)fluoranthene	A	ug/L	4.20937	4.20937		5	0	0	0.0295	0.1	10	84%	44	111	0%	
Chrysene	A	ug/L	4.75365	4.75365		5	0	0	0.0458	0.1	10	95%	50	106	0%	
Dibenzo(a,h)anthracene	A	ug/L	4.69063	4.69063		5	0	0	0.0367	0.1	10	94%	47	111	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15044403	LLCSD-162744	SVOC-8270C-SI	LCSD	√5975.I\sh0113221	13/2022 6:58:0	1	162744	1/6/2022 3:2	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Fluoranthene	A	ug/L	4.26574	4.26574		5	0	0	0.0233	0.1	10	85%	44	111	0%	
Fluorene	A	ug/L	3.90488	3.90488		5	0	0	0.0225	0.1	10	78%	42	99	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	4.87241	4.87241		5	0	0	0.0491	0.1	10	97%	33	112	0%	
Naphthalene	A	ug/L	2.96644	2.96644		5	0	0	0.029	0.1	10	59%	22	108	0%	
Phenanthrene	A	ug/L	4.4789	4.4789		5	0	0	0.0295	0.1	10	90%	43	106	0%	
Pyrene	A	ug/L	4.38756	4.38756		5	0	0	0.0239	0.1	10	88%	41	106	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%				0%
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%				0%
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%				0%
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%				0%
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%				0%
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1	10	0%				0%
2-Fluorobiphenyl	S	ug/L	3.14547	3.14547		5	0	0	0.0444	0.1	10	63%	25	94	0%	
Nitrobenzene-d5	S	ug/L	3.34068	3.34068		5	0	0	0.0523	0.1	10	67%	19	102	0%	
Terphenyl-d14	S	ug/L	4.68188	4.68188		5	0	0	0.0563	0.1	10	94%	39	106	0%	
o-Terphenyl	X	ug/L	3.51466	3.51466		5	0	0	0.0654	0	0	70%	40	140	0%	



Write Sequence

Insert Entries(Have the first cell for entries select)

File Name	Sample Name	Line No.	Test Code	Multiplier	Divisor	Method Name
Jan1301.d	13-Jan-22_TUNE_1	1		1	1	5975Tune.M
Jan1302.d	13-Jan-22_CCV_2	2	SVOC-8270-S-LLPAH	1	1	5975BNASIM.M
Jan1303.d	13-Jan-22_ISTBLK_3	3	SVOC-8270-S-LLPAH	1	1	5975BNASIM.M
Jan1304.d	B22010648-005A	4	SVOC-8270-S-LLPAH	1	1	5975BNASIM.M
Jan1305.d	B22010648-005A	5	SVOC-8270-S-LLPAH	20	1	5975BNASIM.M
Jan1306.d	MB-162744	6	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1307.d	LLCS-162744	7	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1308.d	LLCSD-162744	8	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1309.d	B22010213-001C	9	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1310.d	B22010213-002A	10	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1311.d	B22010213-003C	11	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1312.d	B22010213-003CLMS	12	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1313.d	B22010214-001C	13	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1314.d	B22010219-001C	14	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1315.d	13-Jan-22_CCV_15	15	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1316.d	13-Jan-22_TUNE_16	16		1	1	5975Tune.M
Jan1317.d	13-Jan-22_CCV_17	15	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1318.d	13-Jan-22_ISTBLK_18	18	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1319.d	MB-162910-162494-162167	19	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1320.d	MB-162910-162494-162167	20	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Jan1321.d	LCS-162910-162494-162167	21	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Jan1322.d	B21120800-003D	22	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Jan1323.d	B21120800-003DMS	23	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Jan1324.d	B21120800-003DMSD	24	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Jan1325.d	B21120838-006D	25	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1326.d	B21120838-006D	26	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Jan1327.d	B21120838-007D	27	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1328.d	B21120838-007D	28	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M









Tune Evaluation Report

Data Path: \\MASSHUNTER\Org\Data\SV5975.I\sh011322\1 e8270d bna SIM\Jan1301.D
 Acq on: 1/13/2022 3:19:32 PM
 Operator: LIMS import
 Sample: 13-Jan-22_TUNE_1
 Inst Name: GCMS
 ALS Vial: 1
 Method: \\MASSHUNTER\Org\Data\SV5975.I\Methods\DFTPP5975625.m




Target Mass	Rel. To Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Pass/Fail
51	198	30	60	52.6	141952	Pass
68	69	0	2	0.0	0	Pass
70	69	0	2	0.6	1296	Pass
127	198	40	60	58.2	156864	Pass
197	198	0	1	0.0	0	Pass
198	198	100	100	100.0	269632	Pass
199	198	5	9	7.2	19320	Pass
275	198	10	30	26.5	71360	Pass
365	198	1	100	2.5	6804	Pass
441	443	1E-10	150	92.6	27656	Pass
442	198	40	100	57.9	156224	Pass
443	442	17	23	19.1	29856	Pass
69	69	100	100	100.0	210496	Pass

Tune Evaluation Report



Tune Evaluation Report


+ Scan (rt: 8.181-8.220 min, 28 scans) Jan1301.D 4,4'-DDE




Compound Name	Expected RT	Observed RT	TIC Area	Breakdown %	Pass/Fail
4,4'-DDT	8.800	8.711	4038861	0.5	Pass
4,4'-DDD	8.500	8.407	18651		
4,4'-DDE	8.200	0.000	0		

Tune Evaluation Report

+ Scan (rt: 6.406 min) Jan1301.D Pentachlorophenol



+ Scan (rt: 7.935 min) Jan1301.D Benzidine




Compound Name	Expected RT	Observed RT	Tailing Factor	PGF	Pass/Fail
Pentachlorophenol	6.800	6.406	0.5	3.4	Pass
Benzidine	8.400	7.935	0.2	1.9	Pass

Quantitation Results Report (QT Reviewed)

Data File	Jan1302.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/13/2022 3:43:22 PM
Sample Name	13-Jan-22_CCV_2	Instrument	GCMS
Vial	2	Multiplier	1.00
DA Method File	011222 bna SIM 1.batch.bin	Comment	SVOC-8270-S-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011322 bna SIM 2.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.509	152.0	199419	40.0000	ng/ml	-0.037
M Naphthalene-d8	5.941	136.0	358024	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.000	164.0	192587	40.0000	ng/ml	-0.013
M Phenanthrene-d10	9.780	188.0	407579	40.0000	ng/ml	-0.013
M Chrysene-d12	14.726	240.0	291387	40.0000	ng/ml	-0.038
M Perylene-d12	18.499	264.0	222675	40.0000	ng/ml	-0.025
System Monitoring Compounds						
S Nitrobenzene-d5	5.143	82.0	7755	1.6915	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 33.83%		
S 2-Fluorobiphenyl	7.252	172.0	18211	1.8994	ng/ml	-0.013
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 37.99%		
S o-Terphenyl	10.299	230.0	12364	1.6544	ng/ml	-0.025
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = 33.09%		*
S Terphenyl-d14	12.263	244.0	10629	1.9714	ng/ml	# -0.025
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 39.43%		
Target Compounds						
T Naphthalene	5.953	128.0	23225	1.9319	ng/ml	93
T 2-Methylnaphthalene	6.790	141.0	13417	1.9352	ng/ml	94
T 1-Methylnaphthalene	6.890	141.0	14041	2.1902	ng/ml	95
T Acenaphthylene	7.826	152.0	22827	2.2163	ng/ml	99
T Acenaphthene	8.038	154.0	14858	1.9842	ng/ml	97
T Fluorene	8.673	166.0	17003	1.9842	ng/ml	98
T Phenanthrene	9.805	178.0	24655	1.9930	ng/ml	91
T Anthracene	9.867	178.0	20700	2.0928	ng/ml	95
T Fluoranthene	11.411	202.0	25428	1.8302	ng/ml	93
T Pyrene	11.794	202.0	26952	1.8542	ng/ml	93
T Benzo(a)Anthracene	14.701	228.0	18504	2.1014	ng/ml	98
T Chrysene	14.789	228.0	25198	2.1044	ng/ml	98
T Benzo(b)fluoranthene	17.733	252.0	17327	1.8048	ng/ml	98


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	17.795	252.0	19159	1.9583	ng/ml	97
T Benzo(a)pyrene	18.376	252.0	13482	2.0059	ng/ml	99
T Indeno(1,2,3-cd)pyrene	20.229	276.0	13509	2.0260	ng/ml	97
T Dibenzo(a,h)anthracene	20.303	278.0	15016	1.9385	ng/ml	95
T Benzo(g,h,i)perylene	20.563	276.0	19618	2.0595	ng/ml #	93


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	1.6915	5.14	-0.03	7755	54.0	37.4	21.6	40.2
					128.0	38.9	21.3	39.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	1.9319	5.95	-0.03	23225	102.0	20.0	0.0	46.6
					129.0	11.3	7.6	14.1






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	1.9352	6.79	-0.01	13417	142.0	143.6	103.3	191.8
					115.0	62.2	36.8	68.3






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	2.1902	6.89	-0.01	14041	142.0	103.6	77.9	144.7
					115.0	65.3	44.4	82.5






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	1.8994	7.25	-0.01	18211	171.0	37.4	26.4	49.0















Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthylene	2.2163	7.83	-0.01	22827	153.0	14.4	10.2	18.9



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	1.9842	8.04	-0.01	14858	153.0	111.4	80.3	149.2
					152.0	53.7	38.4	71.4




Quantitation Results Report (QT Reviewed)

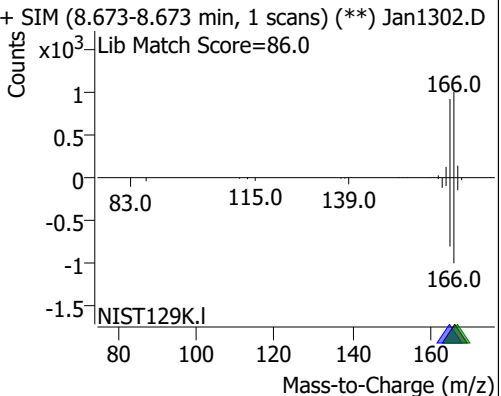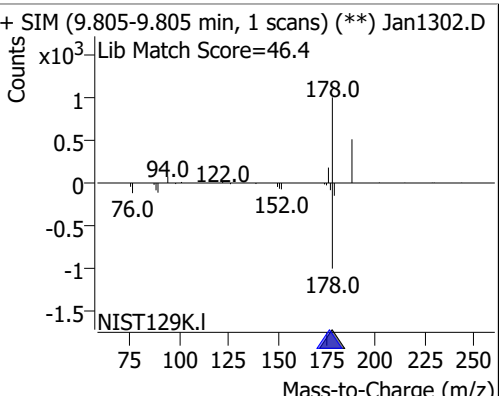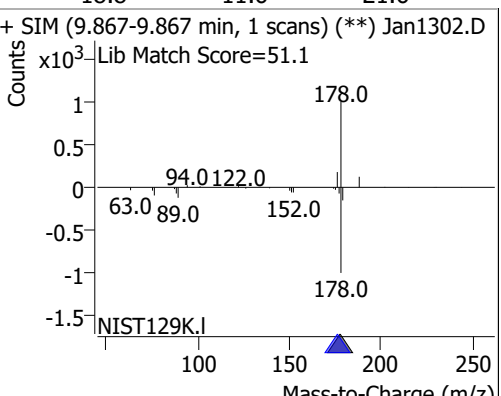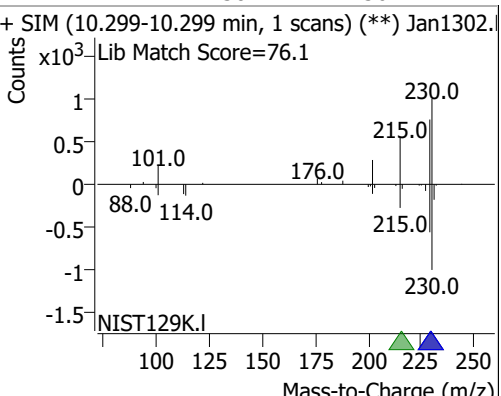
Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene	1.9842	8.67	-0.01	17003	165.0 167.0	98.9 11.8	67.5 7.9	125.3 14.6
+ Selected Ion (166.0) Jan1302.D 			166.0, 165.0, 167.0 			+ SIM (8.673-8.673 min, 1 scans) (**) Jan1302.D Lib Match Score=86.0 		
Phenanthrene	1.9930	9.80	-0.01	24655	176.0	19.1	10.9	20.2
+ Selected Ion (178.0) Jan1302.D 			178.0, 176.0 			+ SIM (9.805-9.805 min, 1 scans) (**) Jan1302.D Lib Match Score=46.4 		
Anthracene	2.0928	9.87	-0.01	20700	176.0	18.8	11.6	21.6
+ Selected Ion (178.0) Jan1302.D 			178.0, 176.0 			+ SIM (9.867-9.867 min, 1 scans) (**) Jan1302.D Lib Match Score=51.1 		
o-Terphenyl	1.6544	10.30	-0.02	12364	229.0 215.0	69.8 47.2	46.7 30.2	86.8 56.2
+ Selected Ion (230.0) Jan1302.D 			230.0, 229.0, 215.0 			+ SIM (10.299-10.299 min, 1 scans) (**) Jan1302.D Lib Match Score=76.1 		

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluoranthene	1.8302	11.41	-0.02	25428	101.0	14.0	8.0	14.8




Pyrene	1.8542	11.79	-0.02	26952	101.0	16.8	9.7	18.1
--------	--------	-------	-------	-------	-------	------	-----	------



Terphenyl-d14	1.9714	12.26	-0.02	10629	122.0	19.4	9.6	17.9
---------------	--------	-------	-------	-------	-------	------	-----	------




Benzo(a)Anthracene	2.1014	14.70	-0.03	18504	226.0	27.1	19.5	36.3
					229.0	22.7	16.5	30.6




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	2.1044	14.79	-0.04	25198	226.0	30.5	22.2	41.2
					229.0	21.2	15.5	28.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(b)fluoranthene	1.8048	17.73	-0.02	17327	253.0	21.6	15.8	29.4



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(k)fluoranthene	1.9583	17.79	-0.02	19159	253.0	21.4	16.1	30.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene	2.0059	18.38	-0.02	13482	253.0	23.1	16.6	30.8




Quantitation Results Report (QT Reviewed)

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Indeno(1,2,3-cd)pyrene	2.0260	20.23	-0.01	13509	138.0	26.6	17.6	32.7
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1302.D</p> </div> <div style="width: 30%;"> <p>276.0, 138.0</p> <p>Ratio = 26.6 (105.6 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.229-20.229 min, 1 scans) (**) Jan1302.D</p> <p>Lib Match Score=75.5</p> </div> </div>								
Dibenzo(a,h)anthracene	1.9385	20.30	-0.01	15016	279.0	24.2	18.1	33.6
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (278.0) Jan1302.D</p> </div> <div style="width: 30%;"> <p>278.0, 279.0, 139.0</p> <p>Ratio = 24.2 (93.4 %)</p> <p>Ratio = 21.8 (119.1 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.303-20.303 min, 1 scans) (**) Jan1302.D</p> <p>Lib Match Score=76.1</p> </div> </div>								
Benzo(g,h,i)perylene	2.0595	20.56	-0.01	19618	277.0	23.5	17.1	31.8
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1302.D</p> </div> <div style="width: 30%;"> <p>276.0, 138.0, 277.0</p> <p>Ratio = 26.1 (130.9 %)</p> <p>Ratio = 23.5 (96.0 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.563-20.563 min, 1 scans) (**) Jan1302.D</p> <p>Lib Match Score=75.6</p> </div> </div>								

Quantitation Results Report (QT Reviewed)

Data File	Jan1303.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/13/2022 4:15:48 PM
Sample Name	13-Jan-22_ISTBLK_3	Instrument	GCMS
Vial	3	Multiplier	1.00
DA Method File	011222 bna SIM 1.batch.bin	Comment	SVOC-8270-S-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011322 bna SIM 2.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library




Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.509	152.0	222112	40.0000	ng/ml	-0.037
M Naphthalene-d8	5.941	136.0	407342	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.001	164.0	227528	40.0000	ng/ml	-0.013
M Phenanthrene-d10	9.780	188.0	459172	40.0000	ng/ml	-0.012
M Chrysene-d12	14.739	240.0	330663	40.0000	ng/ml	# -0.025
M Perylene-d12	18.512	264.0	274843	40.0000	ng/ml	-0.012
System Monitoring Compounds						
S Nitrobenzene-d5	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = NA%		
S 2-Fluorobiphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = NA%		
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = NA%		
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.038	154.0	0		ng/ml md	1
T Fluorene	0.000		0	N.D.		
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	0.000		0	N.D.		
T Chrysene	14.789	228.0	0		ng/ml md	1
T Benzo(b)fluoranthene	0.000		0	N.D.		

Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.388	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)

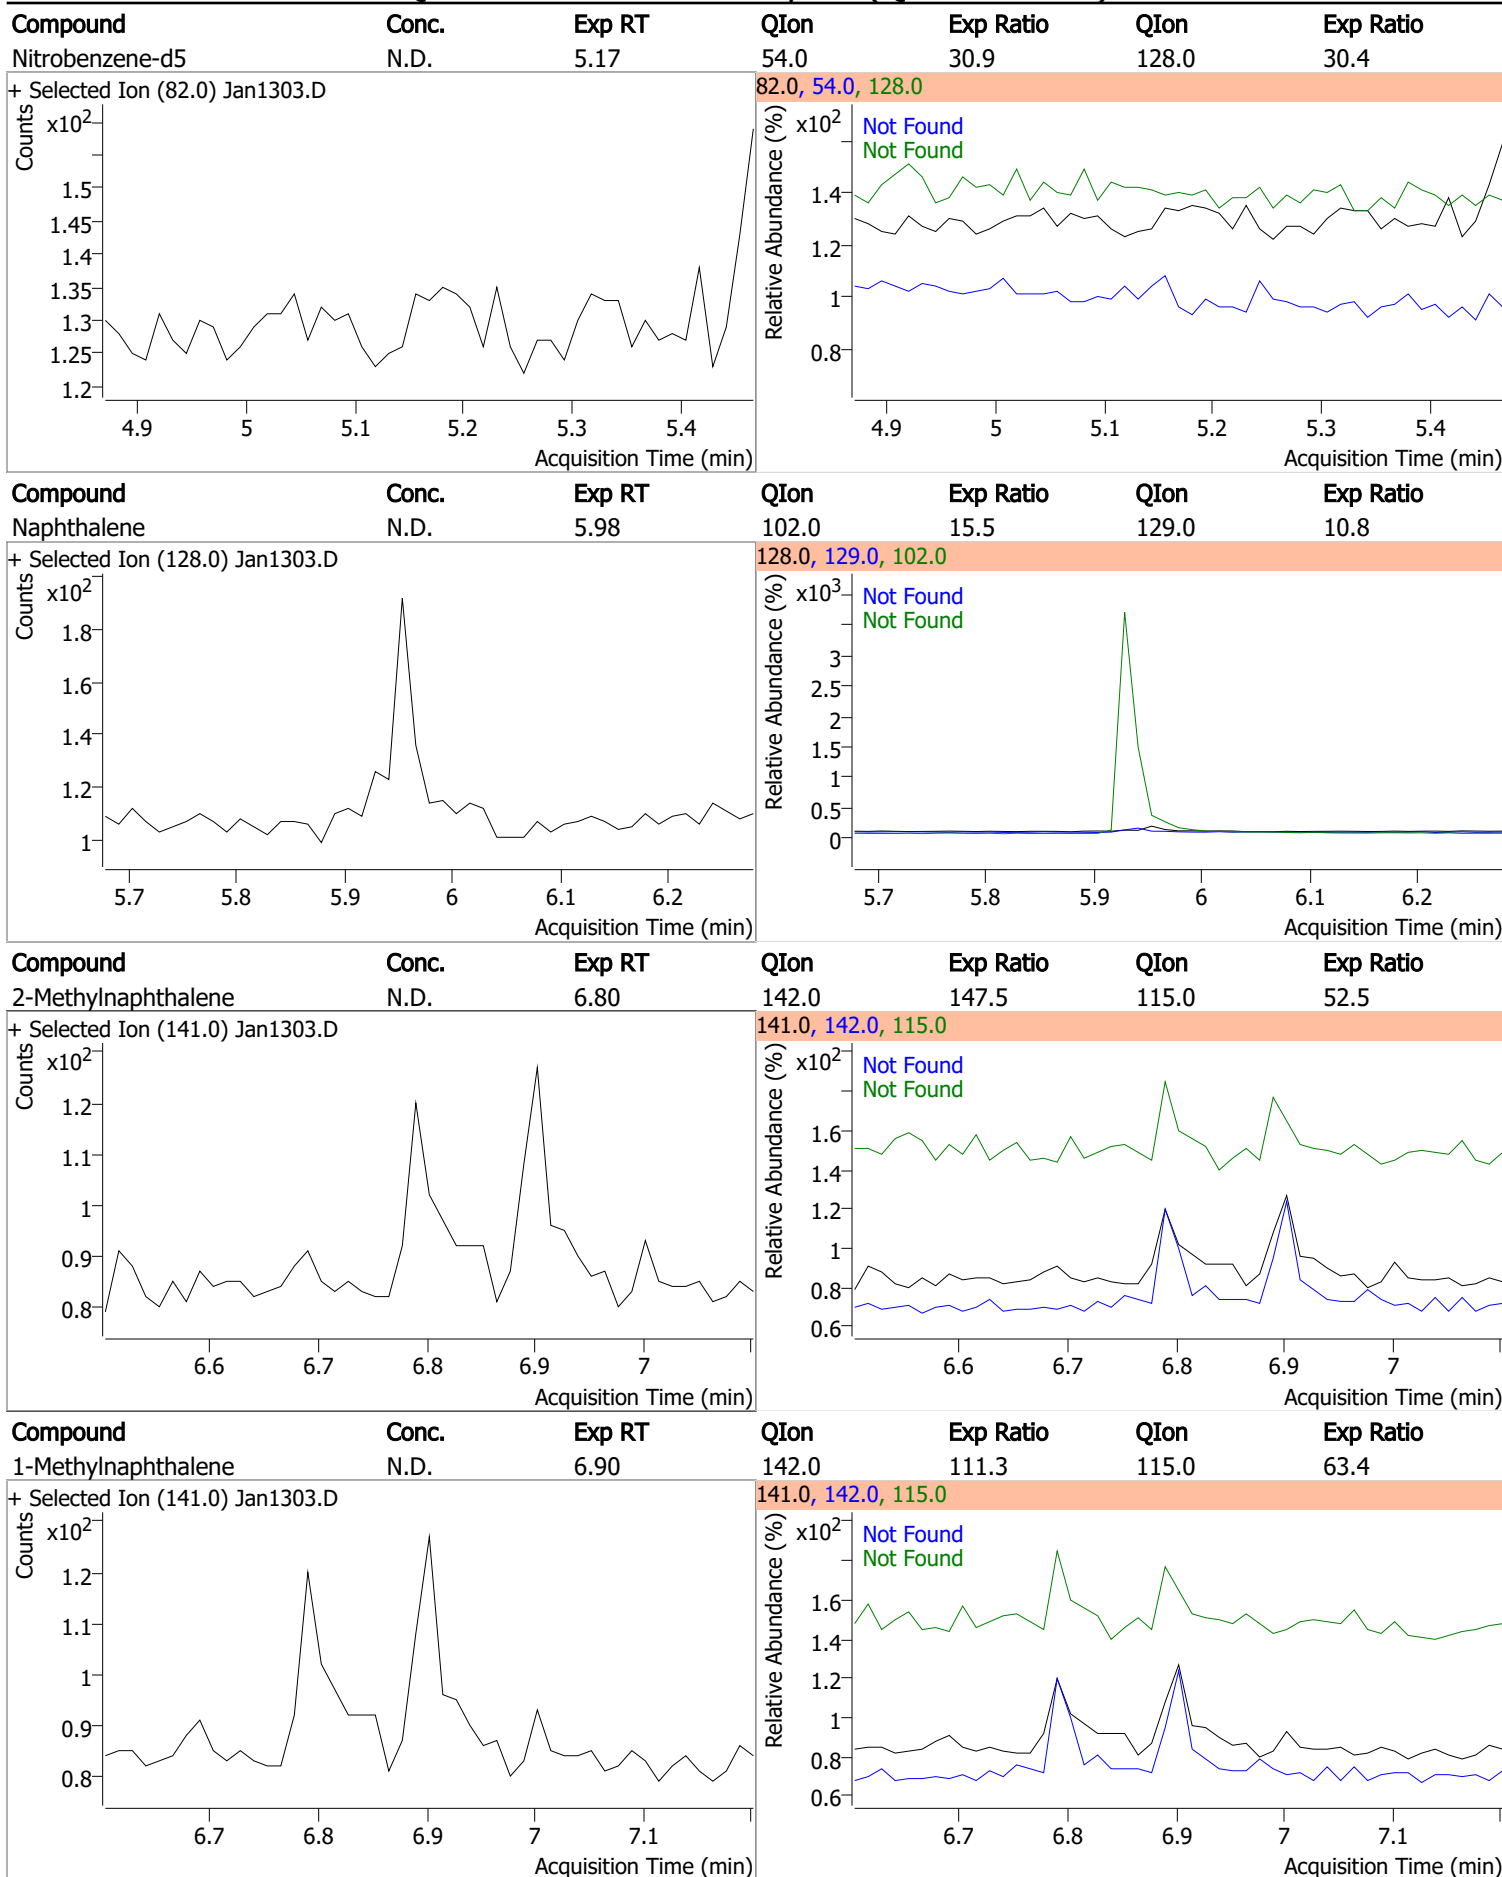


Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
2-Fluorobiphenyl	N.D.	7.26	171.0	37.7




Compound	Conc.	Exp RT	QIon	Exp Ratio
Acenaphthylene	N.D.	7.84	153.0	14.6











Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene		0		0	153.0		80.3	149.2
					152.0		38.4	71.4



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Fluorene	N.D.	8.69	165.0	96.4	167.0	11.3




Quantitation Results Report (QT Reviewed)

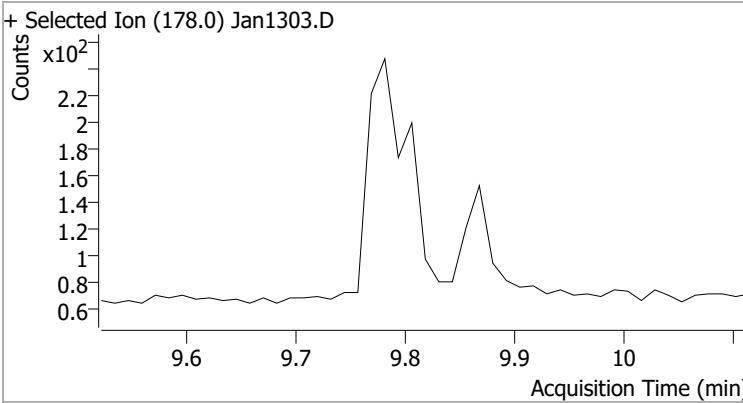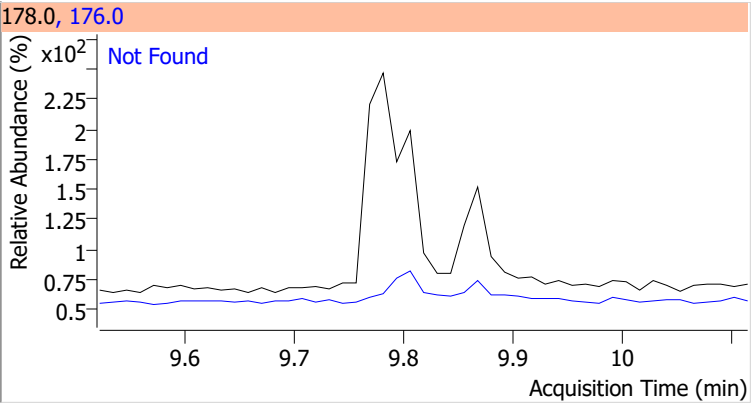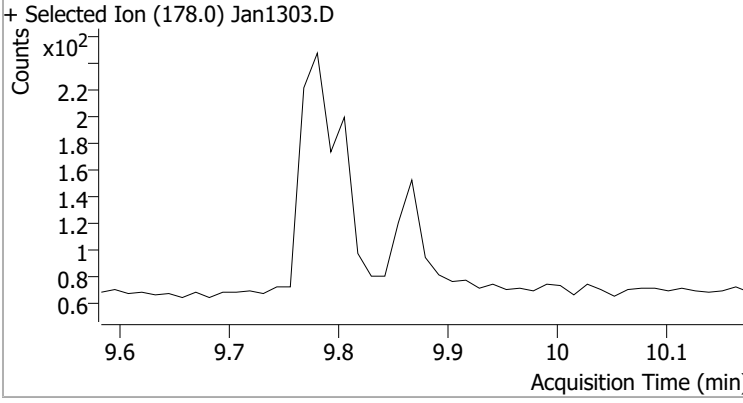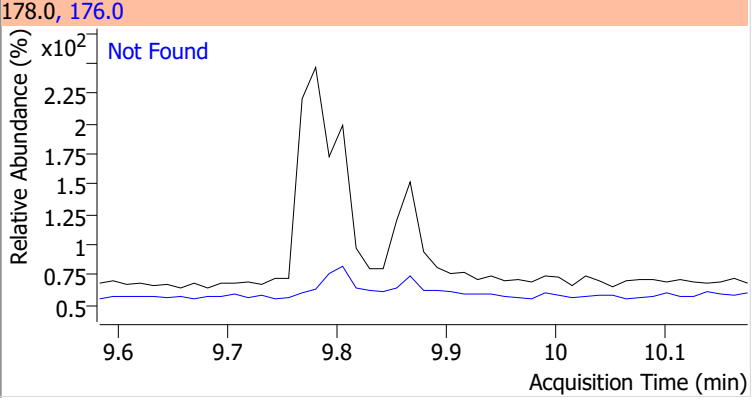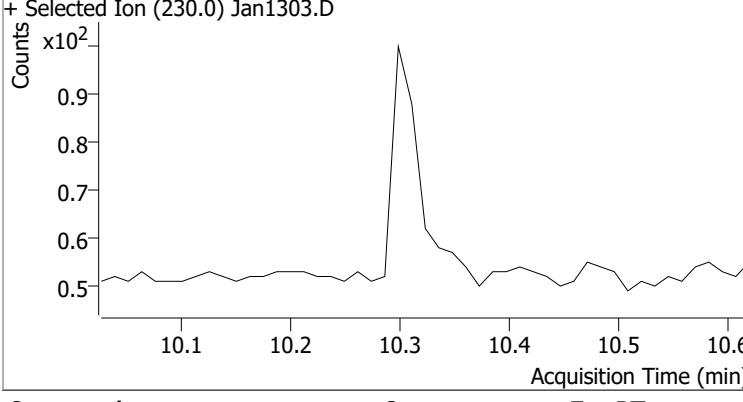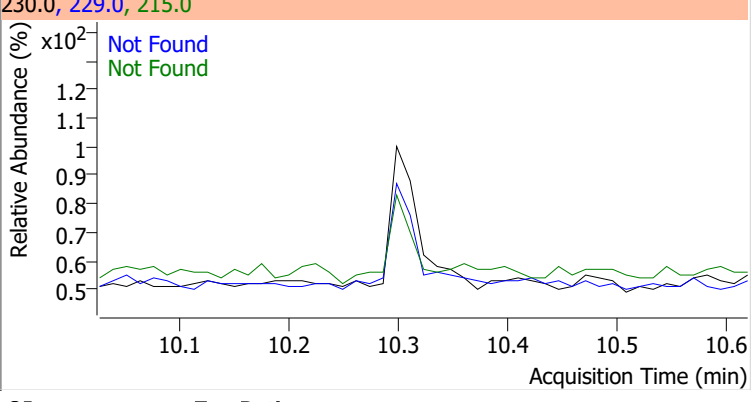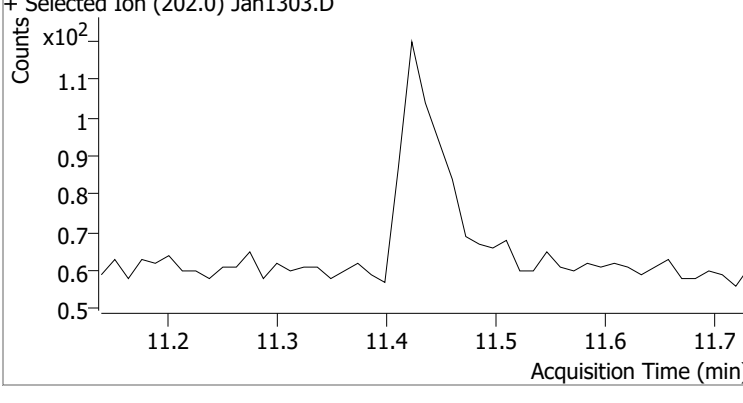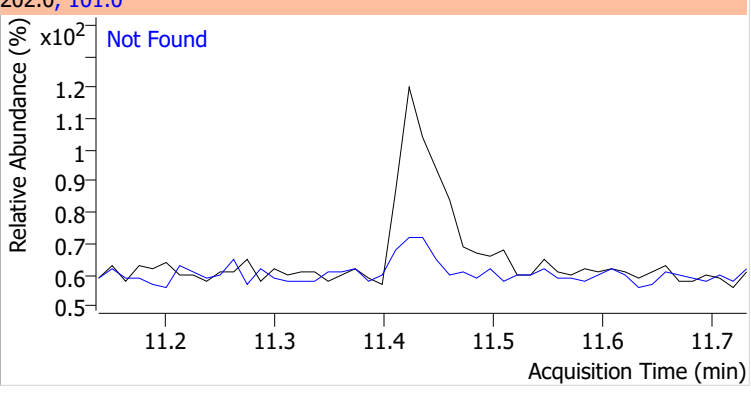
Compound	Conc.	Exp RT	QIon	Exp Ratio		
Phenanthrene	N.D.	9.82	176.0	15.5		
+ Selected Ion (178.0) Jan1303.D 			178.0, 176.0 			
Anthracene	N.D.	9.88	176.0	16.6		
+ Selected Ion (178.0) Jan1303.D 			178.0, 176.0 			
o-Terphenyl	N.D.	10.32	229.0	66.8	QIon	Exp Ratio
			215.0	43.2		
+ Selected Ion (230.0) Jan1303.D 			230.0, 229.0, 215.0 			
Fluoranthene	N.D.	11.44	101.0	11.4		
+ Selected Ion (202.0) Jan1303.D 			202.0, 101.0 			

Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Pyrene	N.D.	11.82	101.0	13.9




Compound	Conc.	Exp RT	QIon	Exp Ratio
Terphenyl-d14	N.D.	12.29	122.0	13.7



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(a)Anthracene	N.D.	14.73	226.0	27.9	229.0	23.5




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene		0		0	226.0		22.2	41.2
					229.0		15.5	28.9




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.6	30.8




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1306.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/13/2022 5:53:11 PM
Sample Name	MB-162744	Instrument	GCMS
Vial	6	Multiplier	1.00
DA Method File	011222 bna SIM 1.batch.bin	Comment	SVOC-8270C-SIM-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011322 bna SIM 2.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.509	152.0	265306	40.0000	ng/ml	-0.037
M Naphthalene-d8	5.941	136.0	466142	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	252339	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.780	188.0	523439	40.0000	ng/ml	-0.012
M Chrysene-d12	14.739	240.0	366496	40.0000	ng/ml	# -0.025
M Perylene-d12	18.512	264.0	302160	40.0000	ng/ml	-0.012
System Monitoring Compounds						
S Nitrobenzene-d5	5.143	82.0	575990	44.4963	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 889.93%		*
S 2-Fluorobiphenyl	7.252	172.0	731766	58.2494	ng/ml	-0.013
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1164.99%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.275	244.0	741601	109.3553	ng/ml	# -0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 2187.11%		*
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.038	154.0	0		ng/ml	md 1
T Fluorene	8.674	166.0	0		ng/ml	md 1
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.739	228.0	0		ng/ml	md 1
T Chrysene	14.801	228.0	0		ng/ml	md 1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.512	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	44.4963	5.14	-0.02	575990	54.0	34.2	21.6	40.2
					128.0	35.8	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4







Quantitation Results Report (QT Reviewed)

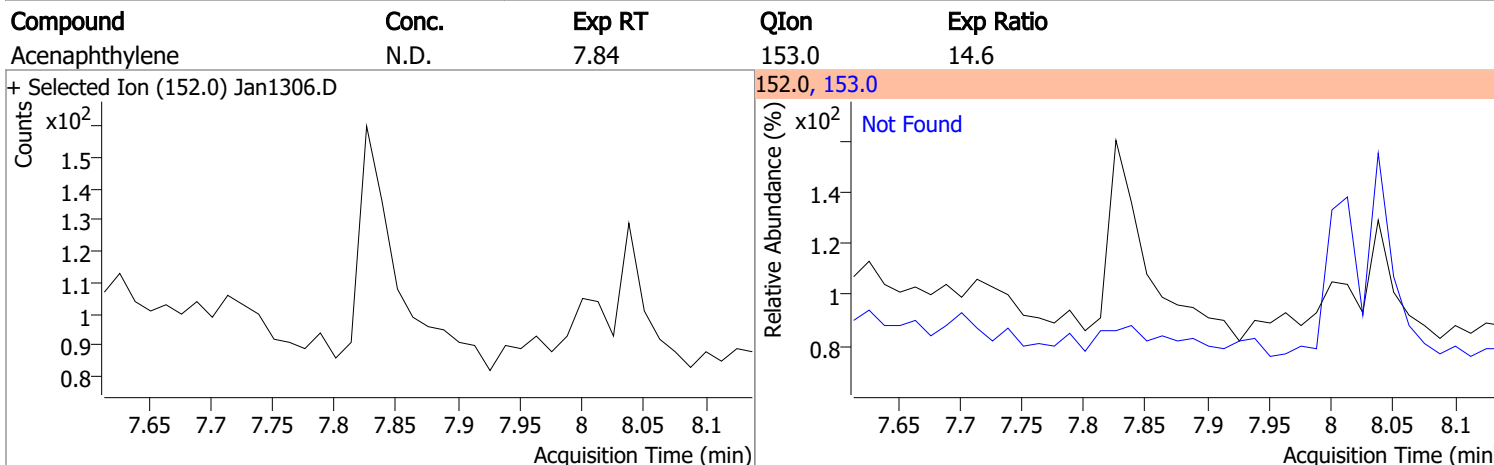

Quantitation Results Report (QT Reviewed)

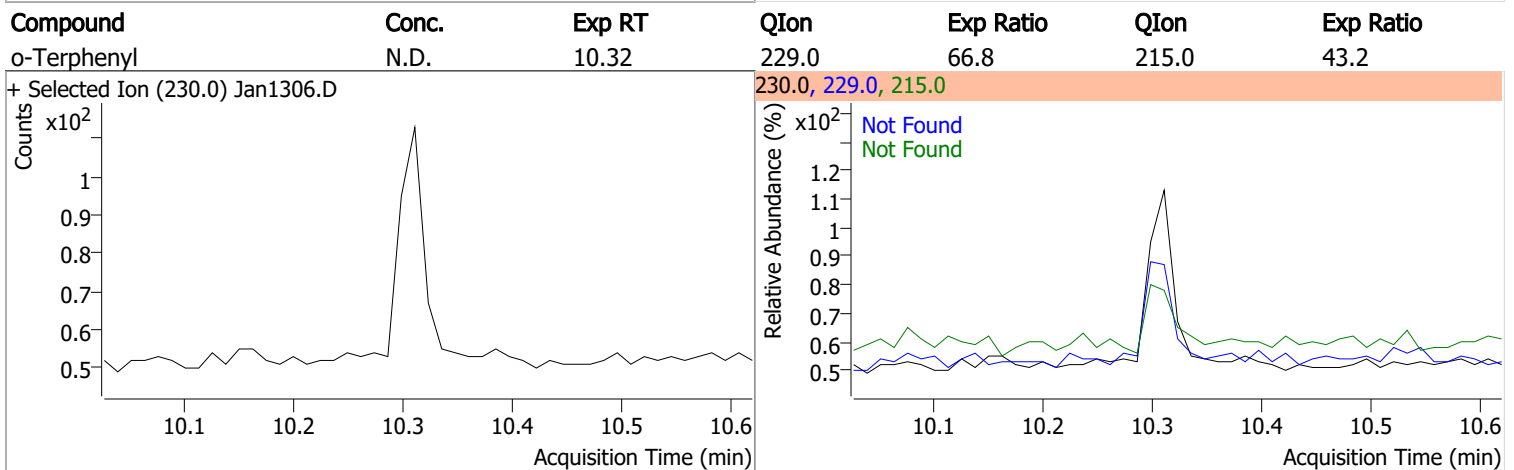


Quantitation Results Report (QT Reviewed)

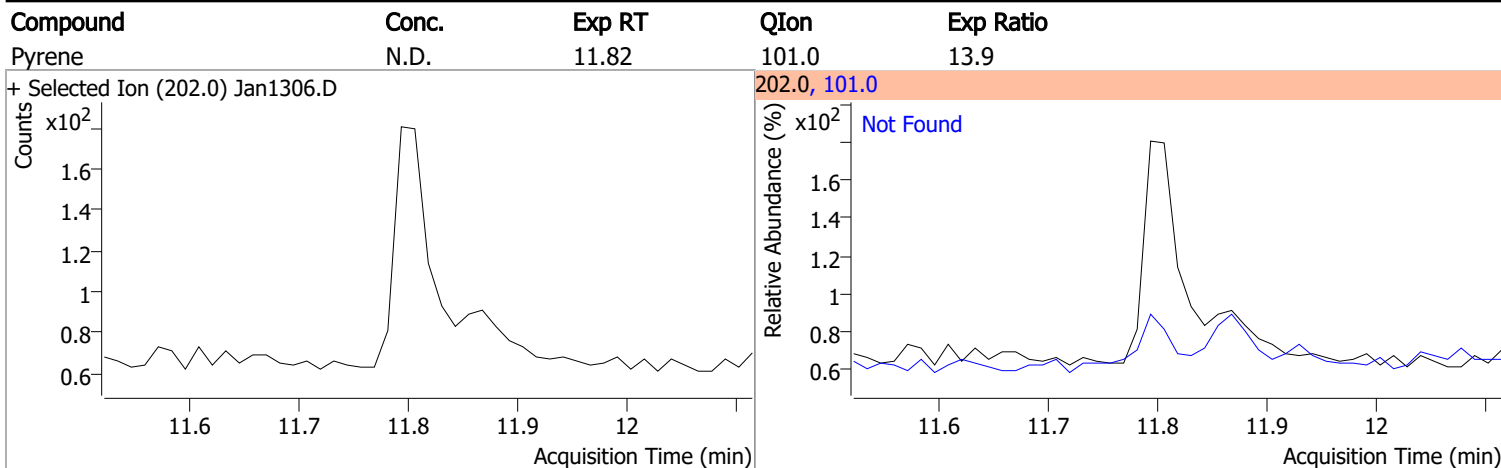


Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.6	30.8




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1307.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/13/2022 6:25:34 PM
Sample Name	LLCS-162744	Instrument	GCMS
Vial	7	Multiplier	1.00
DA Method File	011222 bna SIM 1.batch.bin	Comment	SVOC-8270C-SIM-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011322 bna SIM 2.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.509	152.0	243056	40.0000	ng/ml	-0.038
M Naphthalene-d8	5.941	136.0	440649	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	245162	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.780	188.0	512208	40.0000	ng/ml	-0.013
M Chrysene-d12	14.739	240.0	356471	40.0000	ng/ml	-0.025
M Perylene-d12	18.512	264.0	284847	40.0000	ng/ml	-0.013
System Monitoring Compounds						
S Nitrobenzene-d5	5.143	82.0	20307	3.4550	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 69.10%		
S 2-Fluorobiphenyl	7.252	172.0	40156	3.2901	ng/ml	-0.013
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 65.80%		
S o-Terphenyl	10.299	230.0	30140	3.2091	ng/ml	-0.025
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = 64.18%		
S Terphenyl-d14	12.263	244.0	29989	4.5464	ng/ml	# -0.025
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 90.93%		
Target Compounds						
T Naphthalene	5.953	128.0	50913	3.4409	ng/ml	96
T 2-Methylnaphthalene	6.790	141.0	30015	3.5174	ng/ml	96
T 1-Methylnaphthalene	6.890	141.0	27344	3.4655	ng/ml	m 98
T Acenaphthylene	7.826	152.0	53269	4.0629	ng/ml	98
T Acenaphthene	8.038	154.0	34997	3.6713	ng/ml	95
T Fluorene	8.673	166.0	41202	3.7772	ng/ml	96
T Phenanthrene	9.805	178.0	67330	4.3587	ng/ml	92
T Anthracene	9.867	178.0	60314	4.6678	ng/ml	97
T Fluoranthene	11.411	202.0	70302	4.0265	ng/ml	94
T Pyrene	11.793	202.0	74589	4.1945	ng/ml	95
T Benzo(a)Anthracene	14.714	228.0	52749	4.9088	ng/ml	98
T Chrysene	14.801	228.0	67849	4.5900	ng/ml	97
T Benzo(b)fluoranthene	17.733	252.0	49101	3.9980	ng/ml	99


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	17.795	252.0	52632	4.0461	ng/ml	95
T Benzo(a)pyrene	18.388	252.0	38681	4.2348	ng/ml	100
T Indeno(1,2,3-cd)pyrene	20.229	276.0	41180	4.8280	ng/ml	99
T Dibenzo(a,h)anthracene	20.303	278.0	48533	4.8980	ng/ml	97
T Benzo(g,h,i)perylene	20.563	276.0	59187	4.5702	ng/ml	95


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	3.4550	5.14	-0.03	20307	54.0	35.6	21.6	40.2
					128.0	32.0	21.3	39.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	3.4409	5.95	-0.03	50913	102.0	18.2	0.0	46.6
					129.0	10.9	7.6	14.1




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	3.5174	6.79	-0.01	30015	142.0	148.8	103.3	191.8
					115.0	60.7	36.8	68.3




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	3.4655	6.89	-0.01	27344 (m)	142.0	113.1	77.9	144.7
					115.0	66.3	44.4	82.5




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	3.2901	7.25	-0.01	40156	171.0	36.7	26.4	49.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthylene	4.0629	7.83	-0.01	53269	153.0	13.8	10.2	18.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	3.6713	8.04	-0.01	34997	153.0	118.6	80.3	149.2
					152.0	60.1	38.4	71.4




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene	3.7772	8.67	-0.01	41202	165.0	99.6	67.5	125.3
					167.0	13.7	7.9	14.6




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Phenanthrene	4.3587	9.80	-0.01	67330	176.0	18.8	10.9	20.2



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Anthracene	4.6678	9.87	-0.01	60314	176.0	17.9	11.6	21.6




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
o-Terphenyl	3.2091	10.30	-0.02	30140	229.0	70.6	46.7	86.8
					215.0	47.3	30.2	56.2




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluoranthene	4.0265	11.41	-0.02	70302	101.0	13.6	8.0	14.8




Pyrene	4.1945	11.79	-0.02	74589	101.0	16.1	9.7	18.1
--------	--------	-------	-------	-------	-------	------	-----	------



Terphenyl-d14	4.5464	12.26	-0.02	29989	122.0	19.8	9.6	17.9
---------------	--------	-------	-------	-------	-------	------	-----	------




Benzo(a)Anthracene	4.9088	14.71	-0.01	52749	226.0	27.7	19.5	36.3
					229.0	21.8	16.5	30.6




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	4.5900	14.80	-0.03	67849	226.0	30.2	22.2	41.2
					229.0	21.1	15.5	28.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(b)fluoranthene	3.9980	17.73	-0.02	49101	253.0	22.2	15.8	29.4












Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(k)fluoranthene	4.0461	17.79	-0.02	52632	253.0	20.6	16.1	30.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene	4.2348	18.39	-0.01	38681	253.0	23.8	16.6	30.8




Quantitation Results Report (QT Reviewed)

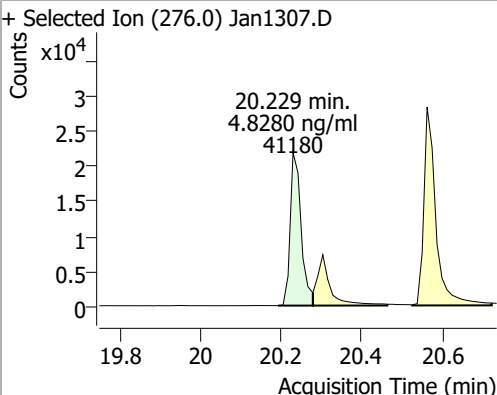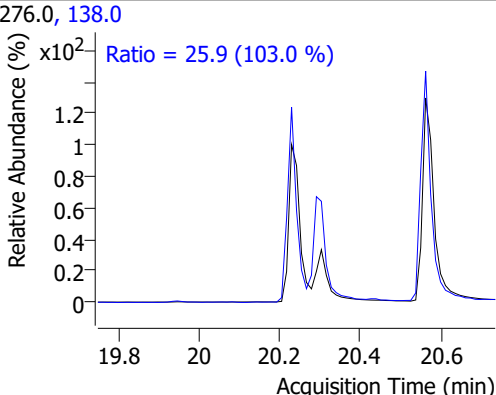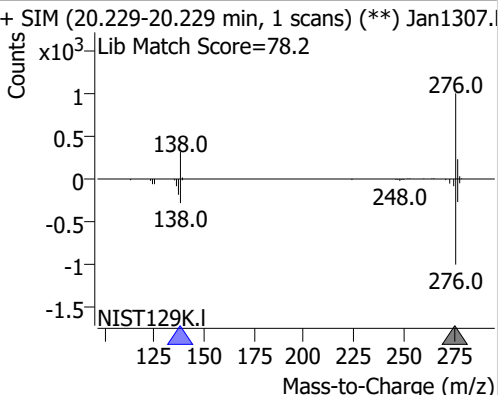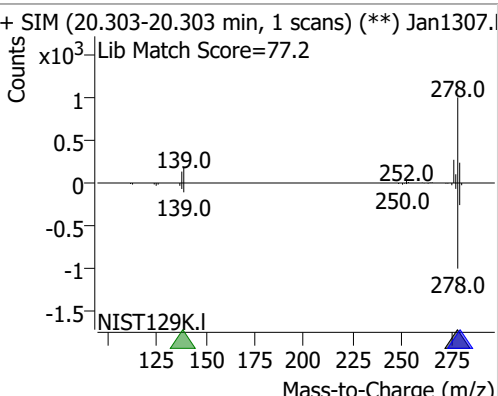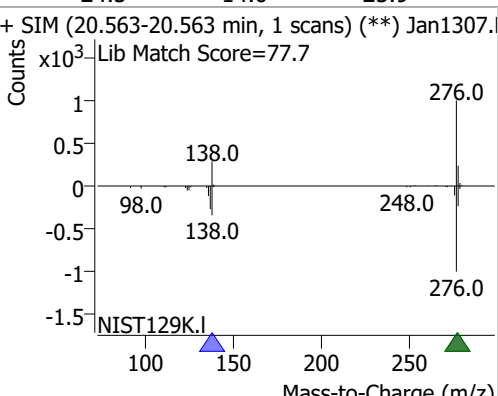Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Indeno(1,2,3-cd)pyrene	4.8280	20.23	-0.01	41180	138.0	25.9	17.6	32.7
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1307.D</p>  </div> <div style="width: 30%;"> <p>276.0, 138.0</p> <p>Ratio = 25.9 (103.0 %)</p>  </div> <div style="width: 30%;"> <p>+ SIM (20.229-20.229 min, 1 scans) (**) Jan1307.D</p> <p>Lib Match Score=78.2</p>  </div> </div>								
Dibenzo(a,h)anthracene	4.8980	20.30	-0.01	48533	279.0	24.3	18.1	33.6
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (278.0) Jan1307.D</p>  </div> <div style="width: 30%;"> <p>278.0, 279.0, 139.0</p> <p>Ratio = 24.3 (94.0 %)</p> <p>Ratio = 19.5 (106.4 %)</p>  </div> <div style="width: 30%;"> <p>+ SIM (20.303-20.303 min, 1 scans) (**) Jan1307.D</p> <p>Lib Match Score=77.2</p>  </div> </div>								
Benzo(g,h,i)perylene	4.5702	20.56	-0.01	59187	277.0	23.6	17.1	31.8
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1307.D</p>  </div> <div style="width: 30%;"> <p>276.0, 138.0, 277.0</p> <p>Ratio = 24.5 (122.9 %)</p> <p>Ratio = 23.6 (96.3 %)</p>  </div> <div style="width: 30%;"> <p>+ SIM (20.563-20.563 min, 1 scans) (**) Jan1307.D</p> <p>Lib Match Score=77.7</p>  </div> </div>								

Quantitation Results Report (QT Reviewed)

Data File	Jan1308.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/13/2022 6:58:07 PM
Sample Name	LLCSD-162744	Instrument	GCMS
Vial	8	Multiplier	1.00
DA Method File	011222 bna SIM 1.batch.bin	Comment	SVOC-8270C-SIM-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011322 bna SIM 2.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.509	152.0	223075	40.0000	ng/ml	-0.037
M Naphthalene-d8	5.941	136.0	413256	40.0000	ng/ml #	-0.013
M Acenaphthene-d10	8.013	164.0	222145	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.780	188.0	462415	40.0000	ng/ml	-0.012
M Chrysene-d12	14.739	240.0	324314	40.0000	ng/ml #	-0.025
M Perylene-d12	18.512	264.0	258540	40.0000	ng/ml	-0.012
System Monitoring Compounds						
S Nitrobenzene-d5	5.143	82.0	17966	3.3407	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 66.81%		
S 2-Fluorobiphenyl	7.252	172.0	34787	3.1455	ng/ml	-0.013
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 62.91%		
S o-Terphenyl	10.299	230.0	29800	3.5147	ng/ml	-0.025
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = 70.29%		
S Terphenyl-d14	12.263	244.0	28096	4.6819	ng/ml #	-0.025
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 93.64%		
Target Compounds						
T Naphthalene	5.953	128.0	41164	2.9664	ng/ml	96
T 2-Methylnaphthalene	6.790	141.0	24101	3.0115	ng/ml m	90
T 1-Methylnaphthalene	6.890	141.0	21191	2.8637	ng/ml m	86
T Acenaphthylene	7.826	152.0	48199	4.0571	ng/ml	97
T Acenaphthene	8.038	154.0	32787	3.7959	ng/ml	97
T Fluorene	8.674	166.0	38596	3.9049	ng/ml	95
T Phenanthrene	9.805	178.0	62463	4.4789	ng/ml	92
T Anthracene	9.867	178.0	55989	4.7893	ng/ml	96
T Fluoranthene	11.411	202.0	67238	4.2657	ng/ml	94
T Pyrene	11.794	202.0	70983	4.3876	ng/ml	94
T Benzo(a)Anthracene	14.714	228.0	49810	5.0874	ng/ml	97
T Chrysene	14.801	228.0	63992	4.7536	ng/ml	98
T Benzo(b)fluoranthene	17.733	252.0	47041	4.2200	ng/ml	98


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	17.795	252.0	49872	4.2094	ng/ml	96
T Benzo(a)pyrene	18.388	252.0	36061	4.3370	ng/ml	100
T Indeno(1,2,3-cd)pyrene	20.229	276.0	37720	4.8724	ng/ml	98
T Dibenzo(a,h)anthracene	20.303	278.0	42186	4.6906	ng/ml	97
T Benzo(g,h,i)perylene	20.563	276.0	55278	4.6885	ng/ml	95


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	3.3407	5.14	-0.02	17966	54.0	36.5	21.6	40.2
					128.0	31.4	21.3	39.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	2.9664	5.95	-0.03	41164	102.0	18.3	0.0	46.6
					129.0	10.8	7.6	14.1




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	3.0115	6.79	-0.01	24101 (m)	142.0	156.9	103.3	191.8
					115.0	63.5	36.8	68.3




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	2.8637	6.89	-0.01	21191 (m)	142.0 115.0	127.0 73.2	77.9 44.4	144.7 82.5




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	3.1455	7.25	-0.01	34787	171.0	36.4	26.4	49.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthylene	4.0571	7.83	-0.01	48199	153.0	13.5	10.2	18.9






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	3.7959	8.04	-0.01	32787	153.0 152.0	116.3 58.5	80.3 38.4	149.2 71.4






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene	3.9049	8.67	-0.01	38596	165.0	101.0	67.5	125.3
					167.0	13.5	7.9	14.6






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Phenanthrene	4.4789	9.81	-0.01	62463	176.0	18.8	10.9	20.2



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Anthracene	4.7893	9.87	-0.01	55989	176.0	18.2	11.6	21.6




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
o-Terphenyl	3.5147	10.30	-0.02	29800	229.0	70.8	46.7	86.8
					215.0	46.9	30.2	56.2




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluoranthene	4.2657	11.41	-0.02	67238	101.0	13.6	8.0	14.8




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Pyrene	4.3876	11.79	-0.02	70983	101.0	16.4	9.7	18.1



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	4.6819	12.26	-0.02	28096	122.0	20.5	9.6	17.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)Anthracene	5.0874	14.71	-0.01	49810	226.0	26.6	19.5	36.3
					229.0	21.7	16.5	30.6




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	4.7536	14.80	-0.02	63992	226.0	30.7	22.2	41.2
					229.0	21.0	15.5	28.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(b)fluoranthene	4.2200	17.73	-0.02	47041	253.0	21.8	15.8	29.4












Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(k)fluoranthene	4.2094	17.80	-0.02	49872	253.0	21.0	16.1	30.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene	4.3370	18.39	-0.01	36061	253.0	23.8	16.6	30.8




Quantitation Results Report (QT Reviewed)

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Indeno(1,2,3-cd)pyrene	4.8724	20.23	-0.01	37720	138.0	26.4	17.6	32.7
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1308.D</p>  </div> <div style="width: 30%;"> <p>276.0, 138.0</p> <p>Ratio = 26.4 (104.9 %)</p>  </div> <div style="width: 30%;"> <p>+ SIM (20.229-20.229 min, 1 scans) (**) Jan1308.I</p> <p>Lib Match Score=78.2</p>  </div> </div>								
Dibenzo(a,h)anthracene	4.6906	20.30	-0.01	42186	279.0	25.9	18.1	33.6
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (278.0) Jan1308.D</p>  </div> <div style="width: 30%;"> <p>278.0, 279.0, 139.0</p> <p>Ratio = 25.9 (100.1 %)</p> <p>Ratio = 21.7 (119.0 %)</p>  </div> <div style="width: 30%;"> <p>+ SIM (20.303-20.303 min, 1 scans) (**) Jan1308.I</p> <p>Lib Match Score=77.4</p>  </div> </div>								
Benzo(g,h,i)perylene	4.6885	20.56	-0.01	55278	277.0	24.0	17.1	31.8
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1308.D</p>  </div> <div style="width: 30%;"> <p>276.0, 138.0, 277.0</p> <p>Ratio = 24.5 (122.7 %)</p> <p>Ratio = 24.0 (98.0 %)</p>  </div> <div style="width: 30%;"> <p>+ SIM (20.563-20.563 min, 1 scans) (**) Jan1308.I</p> <p>Lib Match Score=77.7</p>  </div> </div>								

Quantitation Results Report (QT Reviewed)

Data File	Jan1309.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/13/2022 7:30:30 PM
Sample Name	B22010213-001C	Instrument	GCMS
Vial	9	Multiplier	1.00
DA Method File	011222 bna SIM 1.batch.bin	Comment	SVOC-8270C-SIM-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011322 bna SIM 2.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.509	152.0	234167	40.0000	ng/ml	-0.037
M Naphthalene-d8	5.941	136.0	420729	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	248010	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.780	188.0	515053	40.0000	ng/ml	-0.012
M Chrysene-d12	14.739	240.0	344602	40.0000	ng/ml	# -0.025
M Perylene-d12	18.512	264.0	286787	40.0000	ng/ml	-0.012
System Monitoring Compounds						
S Nitrobenzene-d5	5.131	82.0	516194	44.9372	ng/ml	-0.037
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 898.74%		*
S 2-Fluorobiphenyl	7.265	172.0	662587	53.6633	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1073.27%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.275	244.0	635197	99.6162	ng/ml	# -0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 1992.32%		*
Target Compounds						
T Naphthalene	6.078	128.0	0		ng/ml md	1
T 2-Methylnaphthalene	6.765	141.0	0		ng/ml md	1
T 1-Methylnaphthalene	6.765	141.0	0		ng/ml md	1
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.088	154.0	0		ng/ml md	1
T Fluorene	8.985	166.0	0		ng/ml md	1
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	0.000		0	N.D.		
T Chrysene	14.801	228.0	0		ng/ml md	1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.388	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	44.9372	5.13	-0.04	516194	54.0	34.2	21.6	40.2
					128.0	36.3	21.3	39.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene		0		0	102.0		0.0	46.6
					129.0		7.6	14.1




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene		0		0	142.0		103.3	191.8
					115.0		36.8	68.3




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene		0		0	142.0		77.9	144.7
					115.0		44.4	82.5




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	53.6633	7.26	0.00	662587	171.0	36.5	26.4	49.0



Compound	Conc.	Exp RT	QIon	Exp Ratio
Acenaphthylene	N.D.	7.84	153.0	14.6




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene		0		0	153.0		80.3	149.2
					152.0		38.4	71.4




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene		0		0	165.0 167.0		67.5 7.9	125.3 14.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Phenanthrene	N.D.	9.82	176.0	15.5



Compound	Conc.	Exp RT	QIon	Exp Ratio
Anthracene	N.D.	9.88	176.0	16.6




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
o-Terphenyl	N.D.	10.32	229.0	66.8	215.0	43.2




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Fluoranthene	N.D.	11.44	101.0	11.4




Compound	Conc.	Exp RT	QIon	Exp Ratio
Pyrene	N.D.	11.82	101.0	13.9



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	99.6162	12.28	-0.01	635197	122.0	20.6	9.6	17.9




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(a)Anthracene	N.D.	14.73	226.0	27.9	229.0	23.5




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	0	0		0	226.0		22.2	41.2
					229.0		15.5	28.9




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene	0	0		0	253.0		16.6	30.8




Quantitation Results Report (QT Reviewed)

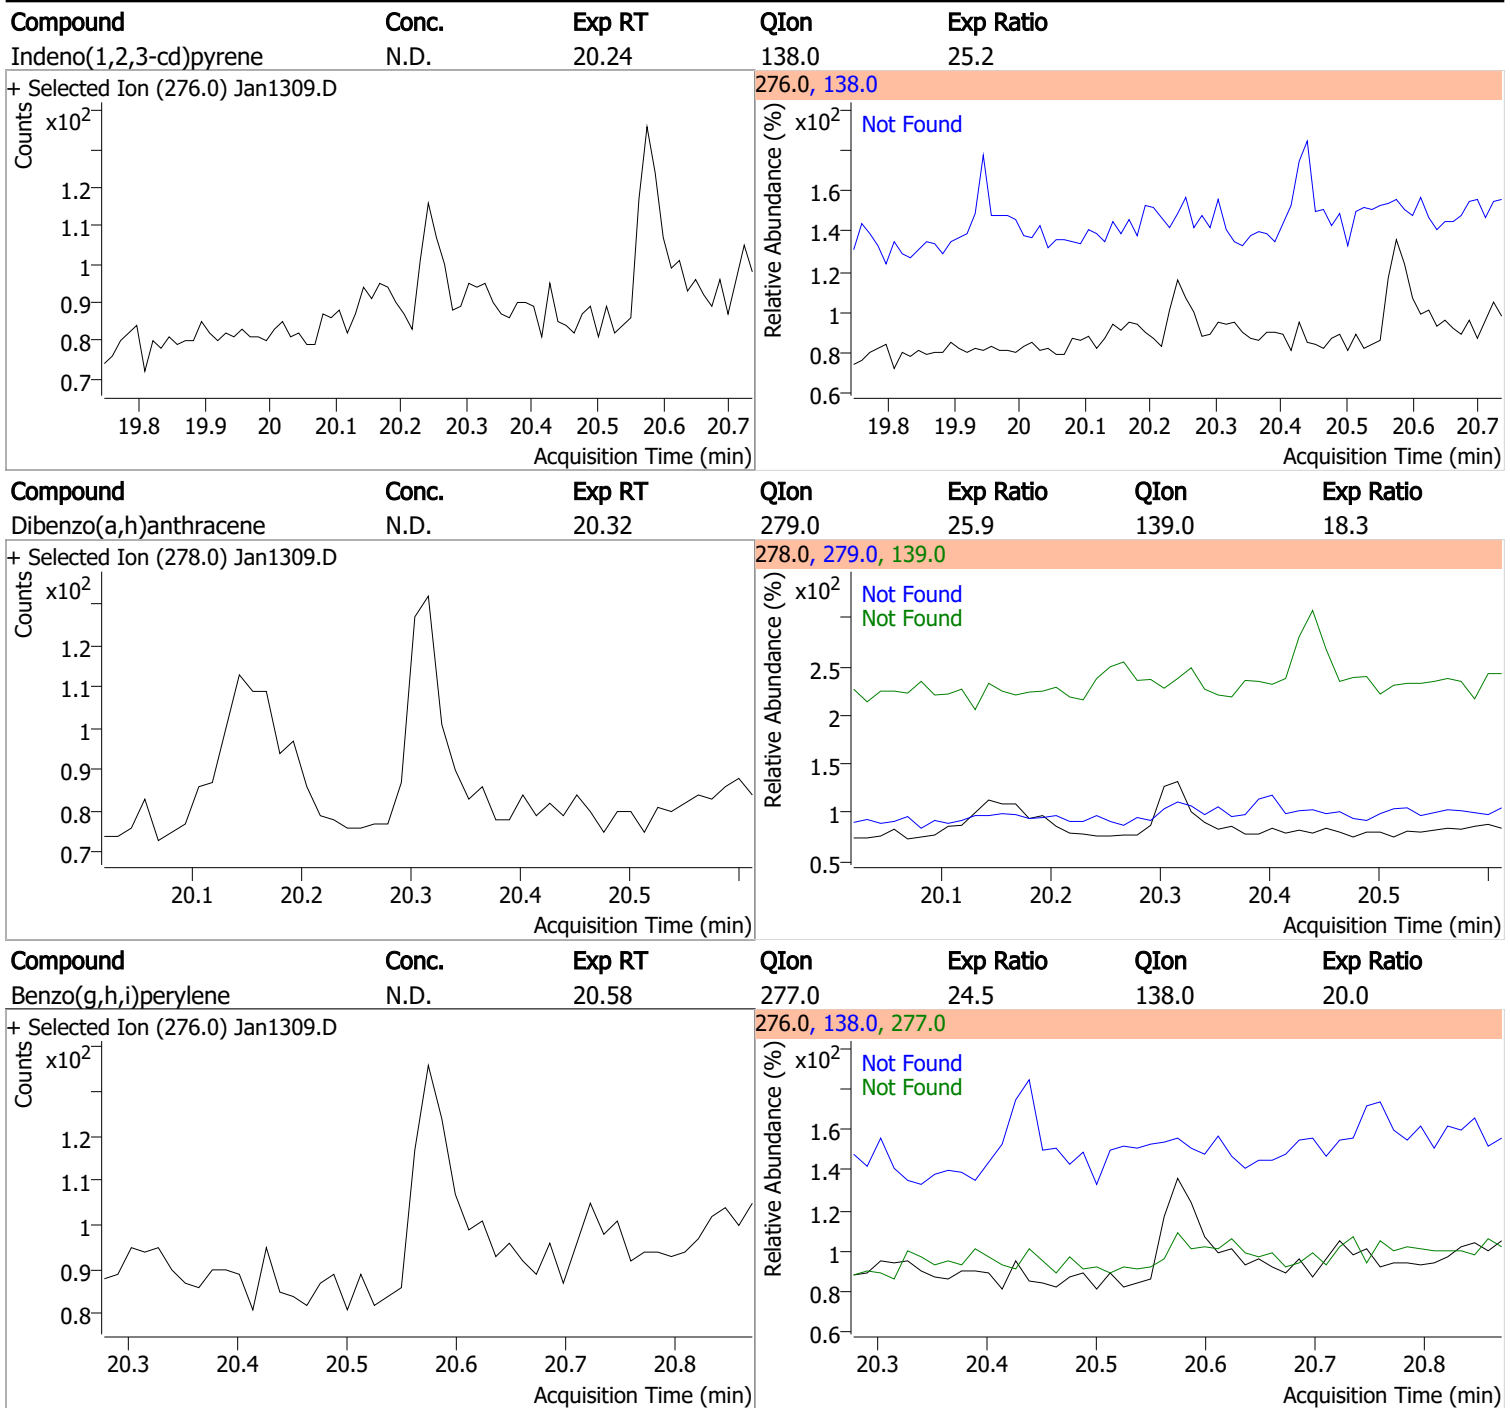

Quantitation Results Report (QT Reviewed)

Data File	Jan1310.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/13/2022 8:03:00 PM
Sample Name	B22010213-002A	Instrument	GCMS
Vial	10	Multiplier	1.00
DA Method File	011222 bna SIM 1.batch.bin	Comment	SVOC-8270C-SIM-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011322 bna SIM 2.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.509	152.0	221989	40.0000	ng/ml	-0.037
M Naphthalene-d8	5.941	136.0	399422	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	228546	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.780	188.0	502389	40.0000	ng/ml	-0.012
M Chrysene-d12	14.739	240.0	327918	40.0000	ng/ml	# -0.025
M Perylene-d12	18.512	264.0	270299	40.0000	ng/ml	-0.012
System Monitoring Compounds						
S Nitrobenzene-d5	5.131	82.0	449990	42.5559	ng/ml	-0.037
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 851.12%		*
S 2-Fluorobiphenyl	7.252	172.0	580848	51.0497	ng/ml	-0.013
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1020.99%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.275	244.0	626777	103.2968	ng/ml	# -0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 2065.94%		*
Target Compounds						
T Naphthalene	6.078	128.0	0		ng/ml	md 1
T 2-Methylnaphthalene	6.765	141.0	0		ng/ml	md 1
T 1-Methylnaphthalene	6.765	141.0	0		ng/ml	md 1
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.038	154.0	0		ng/ml	md 1
T Fluorene	8.674	166.0	0		ng/ml	md 1
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	0.000		0	N.D.		
T Chrysene	14.726	228.0	0		ng/ml	md 1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.512	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	42.5559	5.13	-0.04	449990	54.0	33.8	21.6	40.2
					128.0	33.7	21.3	39.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	0	0	0	0	102.0		0.0	46.6
					129.0		7.6	14.1




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	0	0	0	0	142.0		103.3	191.8
					115.0		36.8	68.3




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene		0		0	142.0		77.9	144.7
					115.0		44.4	82.5




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	51.0497	7.25	-0.01	580848	171.0	37.2	26.4	49.0



Compound	Conc.	Exp RT	QIon	Exp Ratio
Acenaphthylene	N.D.	7.84	153.0	14.6




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene		0		0	153.0		80.3	149.2
					152.0		38.4	71.4




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene		0		0	165.0 167.0		67.5 7.9	125.3 14.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Phenanthrene	N.D.	9.82	176.0	15.5



Compound	Conc.	Exp RT	QIon	Exp Ratio
Anthracene	N.D.	9.88	176.0	16.6




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
o-Terphenyl	N.D.	10.32	229.0	66.8	215.0	43.2




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Fluoranthene	N.D.	11.44	101.0	11.4




Compound	Conc.	Exp RT	QIon	Exp Ratio
Pyrene	N.D.	11.82	101.0	13.9



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	103.2968	12.28	-0.01	626777	122.0	19.4	9.6	17.9




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(a)Anthracene	N.D.	14.73	226.0	27.9	229.0	23.5




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	0	0		0	226.0		22.2	41.2
					229.0		15.5	28.9




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene	0	0		0	253.0		16.6	30.8




Quantitation Results Report (QT Reviewed)

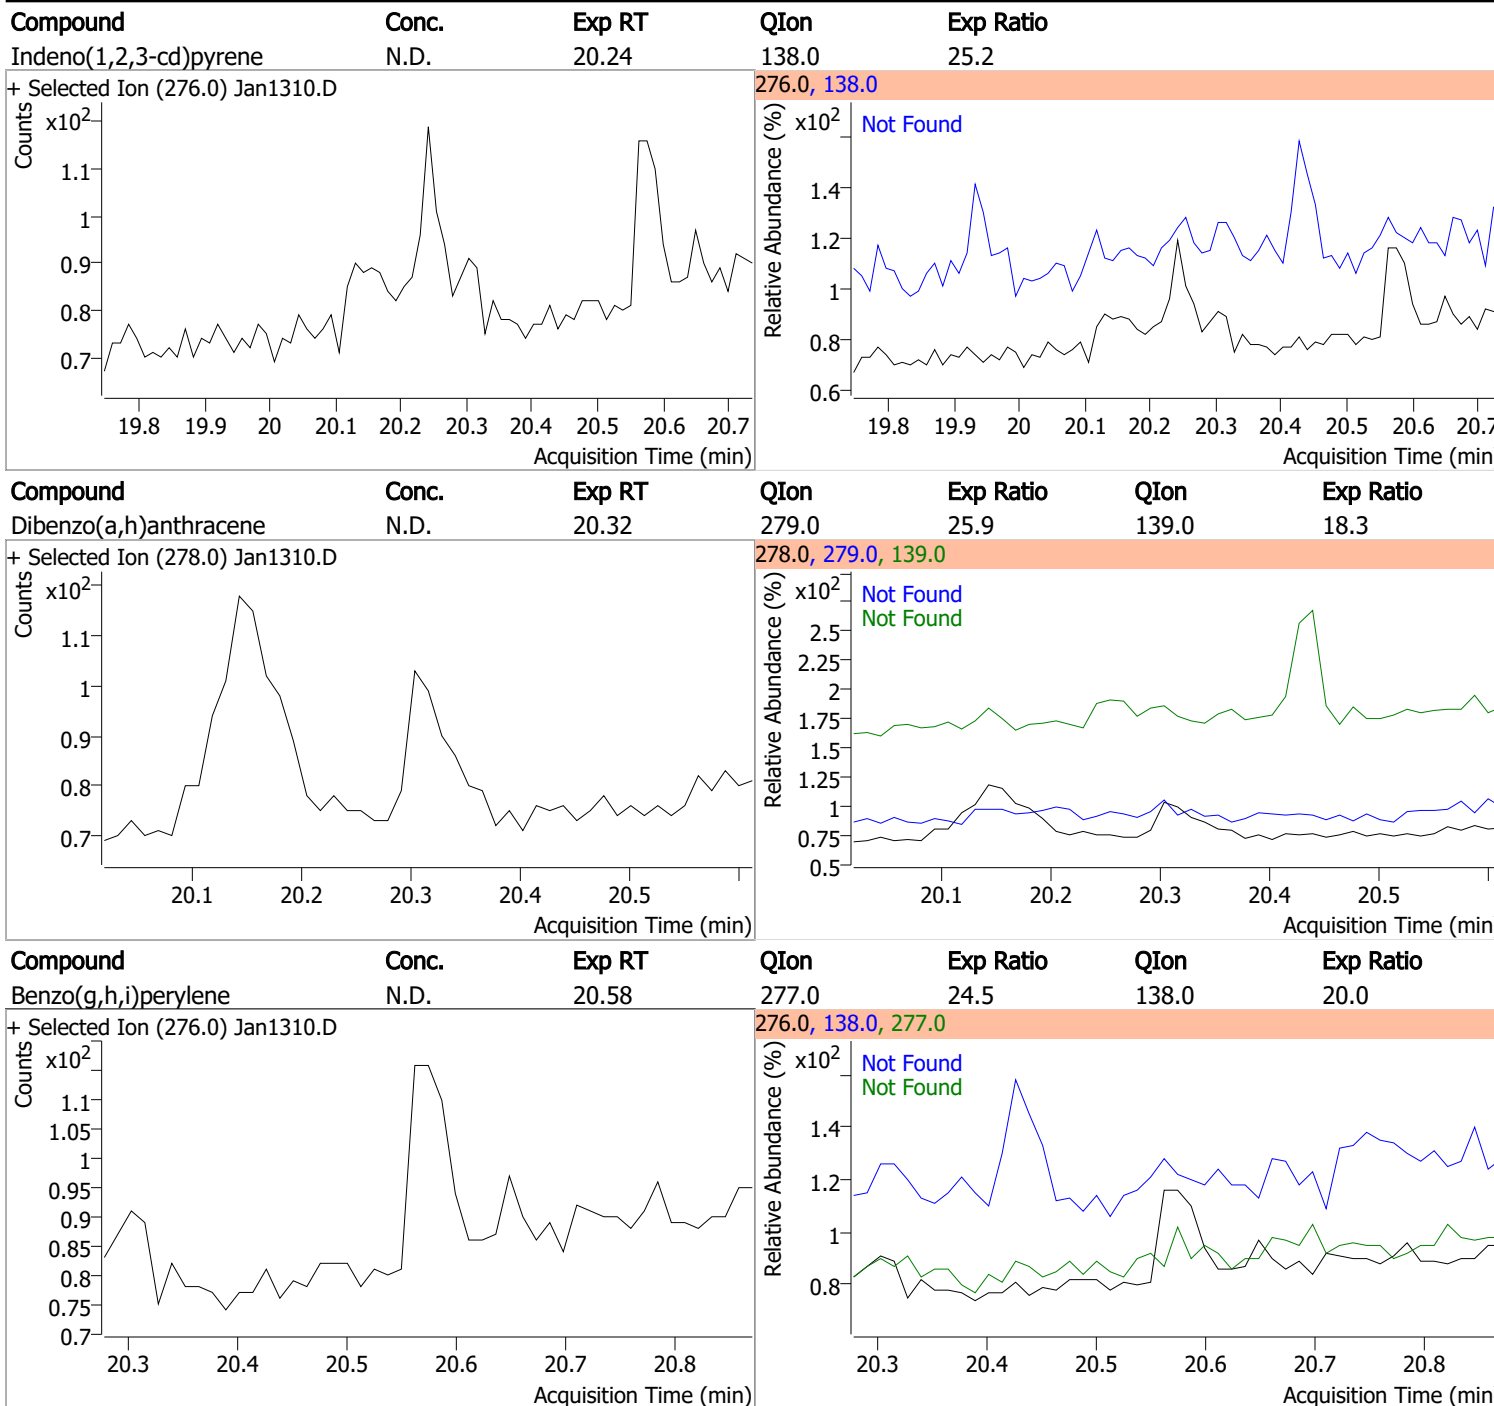

Quantitation Results Report (QT Reviewed)

Data File	Jan1311.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/13/2022 8:35:18 PM
Sample Name	B22010213-003C	Instrument	GCMS
Vial	11	Multiplier	1.00
DA Method File	011222 bna SIM 1.batch.bin	Comment	SVOC-8270C-SIM-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011322 bna SIM 2.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.497	152.0	250070	40.0000	ng/ml	-0.050
M Naphthalene-d8	5.928	136.0	440270	40.0000	ng/ml	-0.025
M Acenaphthene-d10	8.013	164.0	236095	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.780	188.0	515769	40.0000	ng/ml	-0.012
M Chrysene-d12	14.739	240.0	358992	40.0000	ng/ml	# -0.025
M Perylene-d12	18.512	264.0	293310	40.0000	ng/ml	-0.012
System Monitoring Compounds						
S Nitrobenzene-d5	5.131	82.0	474348	40.7462	ng/ml	-0.037
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 814.92%		*
S 2-Fluorobiphenyl	7.252	172.0	552450	47.0013	ng/ml	-0.013
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 940.03%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.275	244.0	633676	95.3942	ng/ml	# -0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 1907.88%		*
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.001	154.0	0		ng/ml	md 1
T Fluorene	8.674	166.0	0		ng/ml	md 1
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.727	228.0	0		ng/ml	md 1
T Chrysene	14.727	228.0	0		ng/ml	md 1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.512	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	40.7462	5.13	-0.04	474348	54.0	36.5	21.6	40.2
					128.0	32.8	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5











Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4







Quantitation Results Report (QT Reviewed)

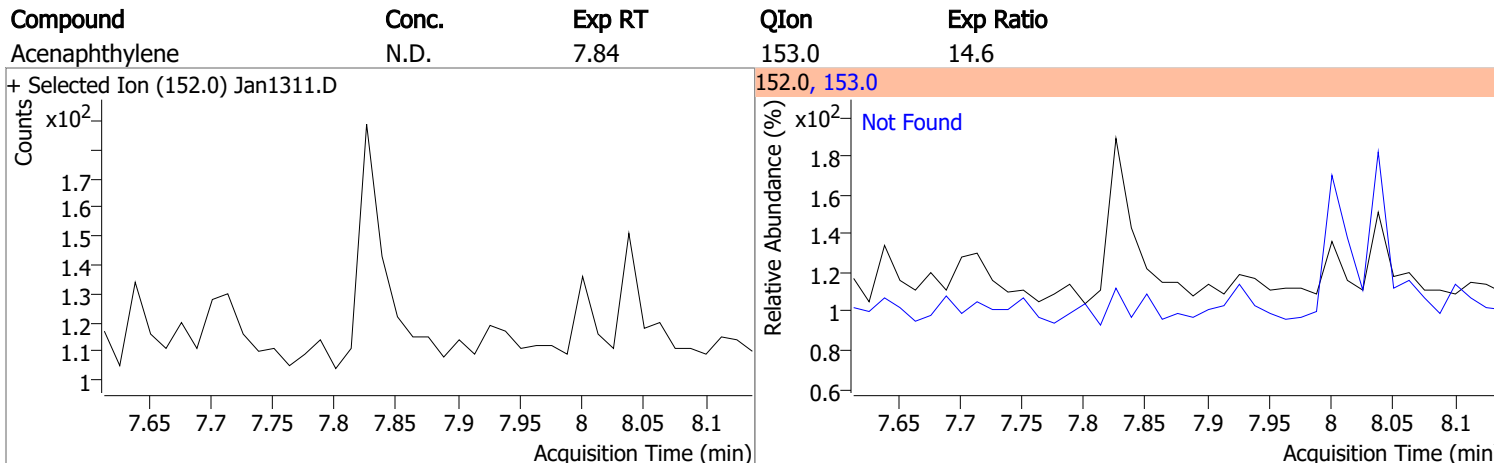

Quantitation Results Report (QT Reviewed)

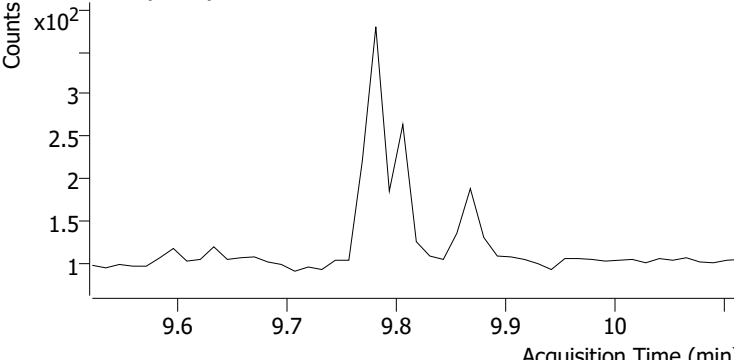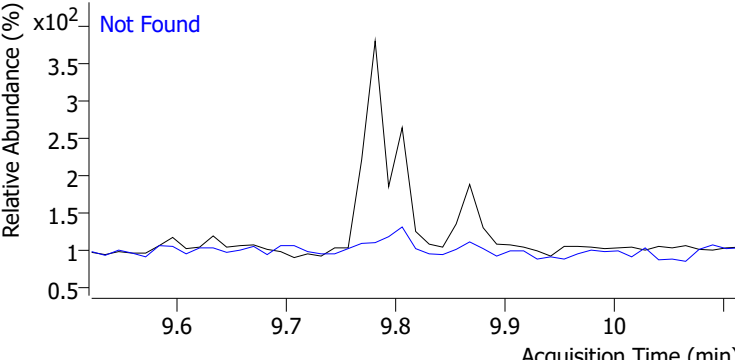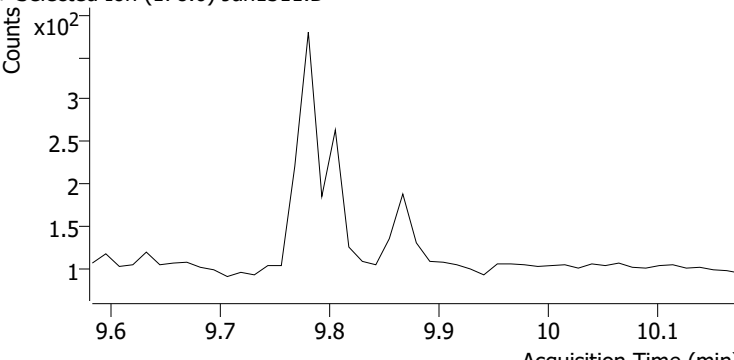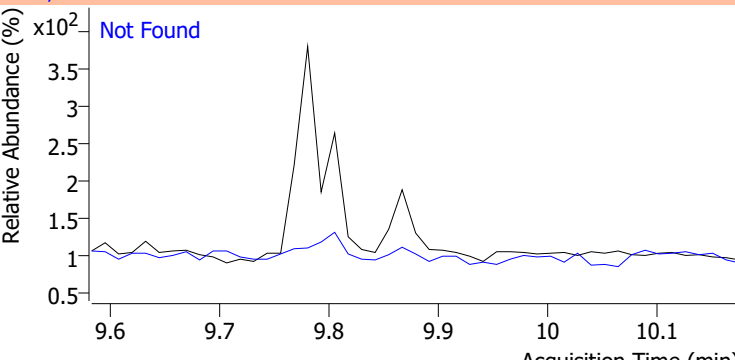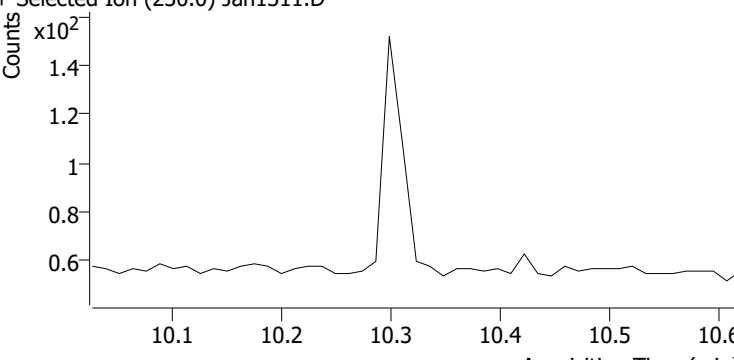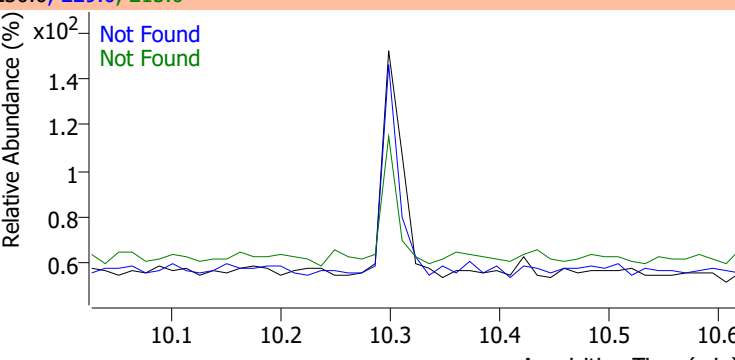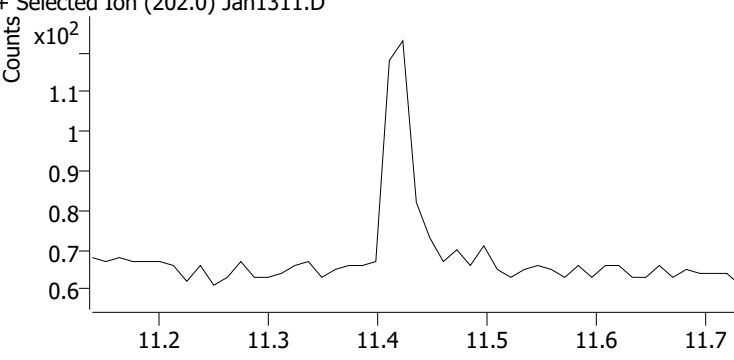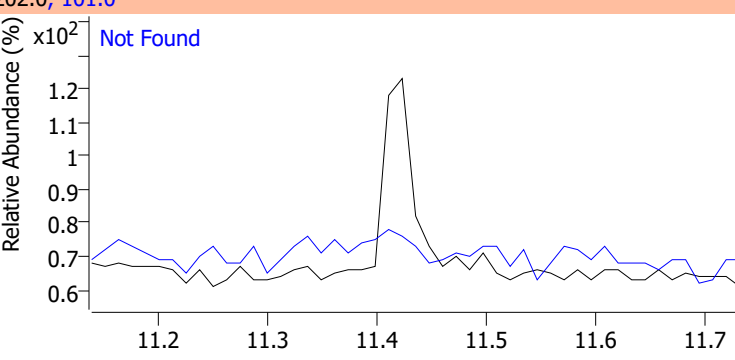
Compound	Conc.	Exp RT	QIon	Exp Ratio		
Phenanthrene	N.D.	9.82	176.0	15.5		
+ Selected Ion (178.0) Jan1311.D			178.0, 176.0			
						
Anthracene	N.D.	9.88	176.0	16.6		
+ Selected Ion (178.0) Jan1311.D			178.0, 176.0			
						
o-Terphenyl	N.D.	10.32	229.0	66.8	QIon	Exp Ratio
					215.0	43.2
+ Selected Ion (230.0) Jan1311.D			230.0, 229.0, 215.0			
						
Fluoranthene	N.D.	11.44	101.0	11.4		
+ Selected Ion (202.0) Jan1311.D			202.0, 101.0			
						

Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.6	30.8




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1312.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/13/2022 9:08:03 PM
Sample Name	B22010213-003CLMS	Instrument	GCMS
Vial	12	Multiplier	1.00
DA Method File	011222 bna SIM 1.batch.bin	Comment	SVOC-8270C-SIM-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011322 bna SIM 2.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.497	152.0	234489	40.0000	ng/ml	-0.050
M Naphthalene-d8	5.928	136.0	424846	40.0000	ng/ml	-0.025
M Acenaphthene-d10	8.000	164.0	243517	40.0000	ng/ml	-0.013
M Phenanthrene-d10	9.780	188.0	496762	40.0000	ng/ml	-0.012
M Chrysene-d12	14.739	240.0	346080	40.0000	ng/ml	# -0.025
M Perylene-d12	18.512	264.0	285376	40.0000	ng/ml	-0.012
System Monitoring Compounds						
S Nitrobenzene-d5	5.131	82.0	20800	3.6497	ng/ml	-0.037
Spiked Amount: 5.000		Range: 19.0 - 102.0%		Recovery = 72.99%		
S 2-Fluorobiphenyl	7.252	172.0	39315	3.2429	ng/ml	-0.013
Spiked Amount: 5.000		Range: 25.0 - 94.0%		Recovery = 64.86%		
S o-Terphenyl	10.299	230.0	30251	3.3211	ng/ml	-0.025
Spiked Amount: 5.000		Range: 40.0 - 140.0%		Recovery = 66.42%		
S Terphenyl-d14	12.263	244.0	28100	4.3880	ng/ml	# -0.025
Spiked Amount: 5.000		Range: 39.0 - 106.0%		Recovery = 87.76%		
Target Compounds						
T Naphthalene	5.953	128.0	41491	2.9084	ng/ml	97
T 2-Methylnaphthalene	6.790	141.0	23462	2.8517	ng/ml	90
T 1-Methylnaphthalene	6.890	141.0	22311	2.9327	ng/ml	96
T Acenaphthylene	7.826	152.0	49661	3.8133	ng/ml	94
T Acenaphthene	8.038	154.0	30309	3.2011	ng/ml	97
T Fluorene	8.673	166.0	37868	3.4949	ng/ml	94
T Phenanthrene	9.805	178.0	52571	3.5080	ng/ml	# 83
T Anthracene	9.867	178.0	56272	4.5034	ng/ml	95
T Fluoranthene	11.411	202.0	68749	4.0600	ng/ml	94
T Pyrene	11.794	202.0	71341	4.1324	ng/ml	93
T Benzo(a)Anthracene	14.701	228.0	51689	4.9527	ng/ml	97
T Chrysene	14.801	228.0	64079	4.4683	ng/ml	98
T Benzo(b)fluoranthene	17.733	252.0	47670	3.8743	ng/ml	100


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	17.795	252.0	47770	3.6930	ng/ml	99
T Benzo(a)pyrene	18.376	252.0	36008	3.9652	ng/ml	99
T Indeno(1,2,3-cd)pyrene	20.229	276.0	37106	4.3424	ng/ml	97
T Dibenzo(a,h)anthracene	20.303	278.0	42533	4.2845	ng/ml	96
T Benzo(g,h,i)perylene	20.563	276.0	51924	4.0551	ng/ml	95


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	3.6497	5.13	-0.04	20800	54.0	37.9	21.6	40.2
					128.0	26.6	21.3	39.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	2.9084	5.95	-0.03	41491	102.0	17.4	0.0	46.6
					129.0	10.7	7.6	14.1




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	2.8517	6.79	-0.01	23462	142.0	158.2	103.3	191.8
					115.0	63.3	36.8	68.3




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	2.9327	6.89	-0.01	22311	142.0	115.7	77.9	144.7
					115.0	67.1	44.4	82.5




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	3.2429	7.25	-0.01	39315	171.0	37.3	26.4	49.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthylene	3.8133	7.83	-0.01	49661	153.0	12.3	10.2	18.9






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	3.2011	8.04	-0.01	30309	153.0	116.7	80.3	149.2
					152.0	58.6	38.4	71.4






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene	3.4949	8.67	-0.01	37868	165.0	102.0	67.5	125.3
					167.0	13.4	7.9	14.6






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Phenanthrene	3.5080	9.80	-0.01	52571	176.0	22.7	10.9	20.2



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Anthracene	4.5034	9.87	-0.01	56272	176.0	18.6	11.6	21.6




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
o-Terphenyl	3.3211	10.30	-0.02	30251	229.0	70.6	46.7	86.8
					215.0	48.0	30.2	56.2




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluoranthene	4.0600	11.41	-0.02	68749	101.0	13.5	8.0	14.8




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Pyrene	4.1324	11.79	-0.02	71341	101.0	16.8	9.7	18.1



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	4.3880	12.26	-0.02	28100	122.0	19.4	9.6	17.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)Anthracene	4.9527	14.70	-0.03	51689	226.0	26.9	19.5	36.3
					229.0	21.7	16.5	30.6




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	4.4683	14.80	-0.03	64079	226.0	30.6	22.2	41.2
					229.0	20.8	15.5	28.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(b)fluoranthene	3.8743	17.73	-0.02	47670	253.0	22.4	15.8	29.4



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(k)fluoranthene	3.6930	17.80	-0.02	47770	253.0	22.7	16.1	30.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene	3.9652	18.38	-0.02	36008	253.0	23.2	16.6	30.8




Quantitation Results Report (QT Reviewed)

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Indeno(1,2,3-cd)pyrene	4.3424	20.23	-0.01	37106	138.0	26.5	17.6	32.7
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1312.D</p> </div> <div style="width: 30%;"> <p>276.0, 138.0</p> <p>Ratio = 26.5 (105.2 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.229-20.229 min, 1 scans) (**) Jan1312.D</p> <p>Lib Match Score=78.6</p> </div> </div>								
Dibenzo(a,h)anthracene	4.2845	20.30	-0.01	42533	279.0	24.8	18.1	33.6
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (278.0) Jan1312.D</p> </div> <div style="width: 30%;"> <p>278.0, 279.0, 139.0</p> <p>Ratio = 24.8 (95.8 %)</p> <p>Ratio = 20.8 (113.6 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.303-20.303 min, 1 scans) (**) Jan1312.D</p> <p>Lib Match Score=77.7</p> </div> </div>								
Benzo(g,h,i)perylene	4.0551	20.56	-0.01	51924	277.0	24.1	17.1	31.8
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1312.D</p> </div> <div style="width: 30%;"> <p>276.0, 138.0, 277.0</p> <p>Ratio = 24.6 (123.4 %)</p> <p>Ratio = 24.1 (98.5 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.563-20.563 min, 1 scans) (**) Jan1312.D</p> <p>Lib Match Score=78.2</p> </div> </div>								

Quantitation Results Report (QT Reviewed)

Data File	Jan1313.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/13/2022 9:40:28 PM
Sample Name	B22010214-001C	Instrument	GCMS
Vial	13	Multiplier	1.00
DA Method File	011222 bna SIM 1.batch.bin	Comment	SVOC-8270C-SIM-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011322 bna SIM 2.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.509	152.0	225686	40.0000	ng/ml	-0.037
M Naphthalene-d8	5.941	136.0	416075	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	226759	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.780	188.0	482602	40.0000	ng/ml	-0.012
M Chrysene-d12	14.739	240.0	340278	40.0000	ng/ml	# -0.025
M Perylene-d12	18.512	264.0	276571	40.0000	ng/ml	-0.012
System Monitoring Compounds						
S Nitrobenzene-d5	5.131	82.0	422435	40.3913	ng/ml	-0.037
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 807.83%		*
S 2-Fluorobiphenyl	7.252	172.0	596658	52.8523	ng/ml	-0.013
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1057.05%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.275	244.0	619160	98.3350	ng/ml	# -0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 1966.70%		*
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.038	154.0	0		ng/ml md	1
T Fluorene	8.973	166.0	0		ng/ml md	1
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	0.000		0	N.D.		
T Chrysene	14.739	228.0	0		ng/ml md	1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.512	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	40.3913	5.13	-0.04	422435	54.0	36.0	21.6	40.2
					128.0	33.3	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4



Quantitation Results Report (QT Reviewed)

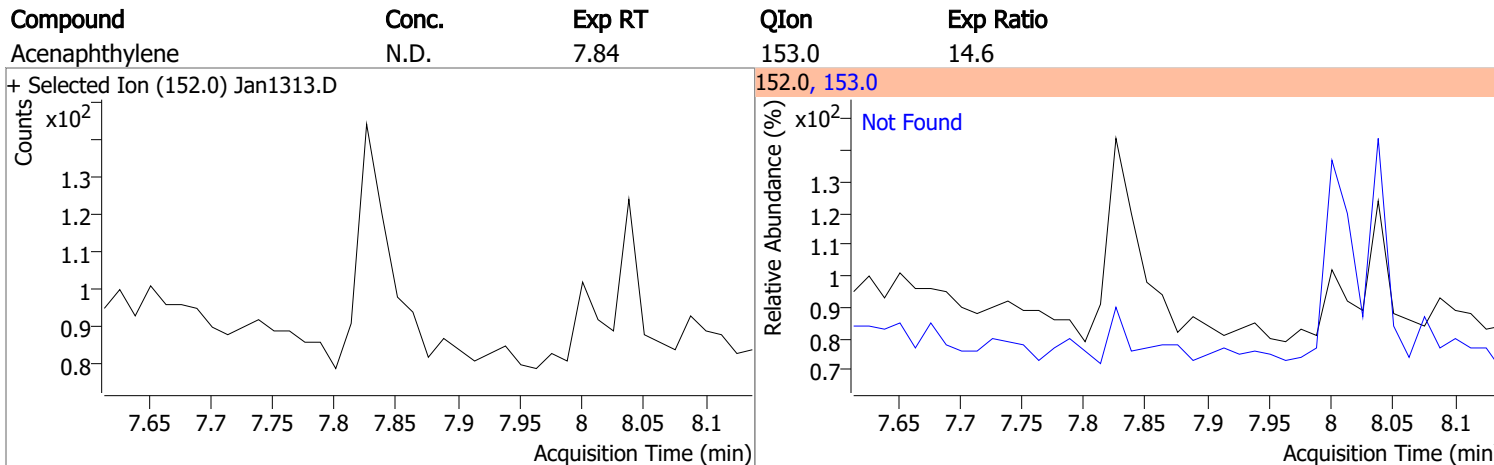


Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio		
Phenanthrene	N.D.	9.82	176.0	15.5		
+ Selected Ion (178.0) Jan1313.D 			178.0, 176.0 			
Anthracene	N.D.	9.88	176.0	16.6		
+ Selected Ion (178.0) Jan1313.D 			178.0, 176.0 			
o-Terphenyl	N.D.	10.32	229.0	66.8	QIon	Exp Ratio
			215.0	43.2		
+ Selected Ion (230.0) Jan1313.D 			230.0, 229.0, 215.0 			
Fluoranthene	N.D.	11.44	101.0	11.4		
+ Selected Ion (202.0) Jan1313.D 			202.0, 101.0 			

Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Pyrene	N.D.	11.82	101.0	13.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	98.3350	12.28	-0.01	619160	122.0	20.7	9.6	17.9



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(a)Anthracene	N.D.	14.73	226.0	27.9	229.0	23.5




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	0	0		0	226.0		22.2	41.2
					229.0		15.5	28.9




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.6	30.8




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1314.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/13/2022 10:12:54 PM
Sample Name	B22010219-001C	Instrument	GCMS
Vial	14	Multiplier	1.00
DA Method File	011222 bna SIM 1.batch.bin	Comment	SVOC-8270C-SIM-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011322 bna SIM 2.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.497	152.0	224313	40.0000	ng/ml	-0.050
M Naphthalene-d8	5.941	136.0	418654	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.013	164.0	229996	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.780	188.0	489287	40.0000	ng/ml	-0.013
M Chrysene-d12	14.739	240.0	339794	40.0000	ng/ml	# -0.025
M Perylene-d12	18.512	264.0	278028	40.0000	ng/ml	-0.013
System Monitoring Compounds						
S Nitrobenzene-d5	5.131	82.0	441562	41.7486	ng/ml	-0.037
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 834.97%		*
S 2-Fluorobiphenyl	7.252	172.0	641091	55.9890	ng/ml	-0.013
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1119.78%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.275	244.0	617061	98.1411	ng/ml	# -0.013
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 1962.82%		*
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.038	154.0	0		ng/ml	md 1
T Fluorene	8.661	166.0	0		ng/ml	md 1
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	0.000		0	N.D.		
T Chrysene	14.739	228.0	0		ng/ml	md 1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.512	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	41.7486	5.13	-0.04	441562	54.0	36.8	21.6	40.2
					128.0	33.5	21.3	39.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.98	102.0	15.5	129.0	10.8



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.80	142.0	147.5	115.0	52.5




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	111.3	115.0	63.4




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	55.9890	7.25	-0.01	641091	171.0	37.4	26.4	49.0




Compound	Conc.	Exp RT	QIon	Exp Ratio
Acenaphthylene	N.D.	7.84	153.0	14.6







Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene		0		0	153.0		80.3	149.2
					152.0		38.4	71.4







Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene		0		0	165.0		67.5	125.3
					167.0		7.9	14.6



Quantitation Results Report (QT Reviewed)

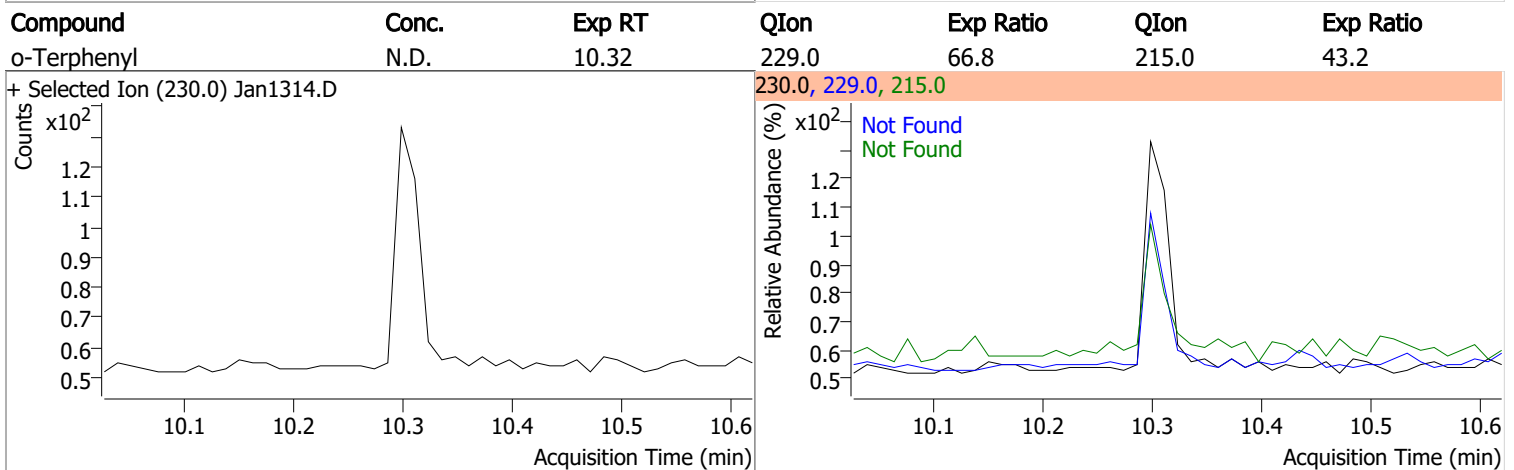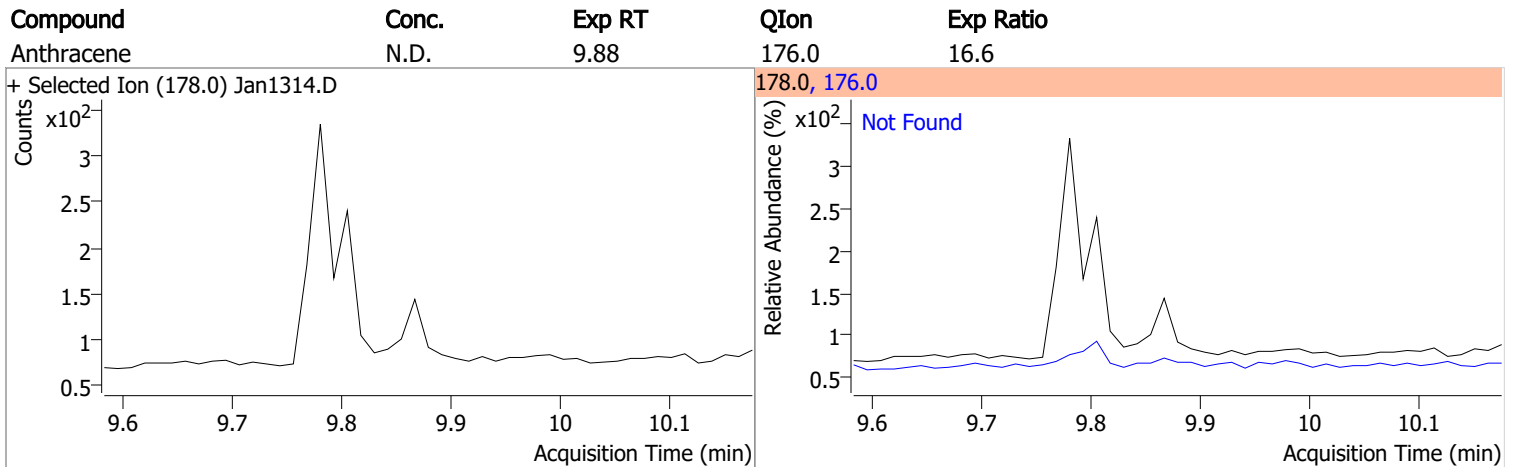


Quantitation Results Report (QT Reviewed)

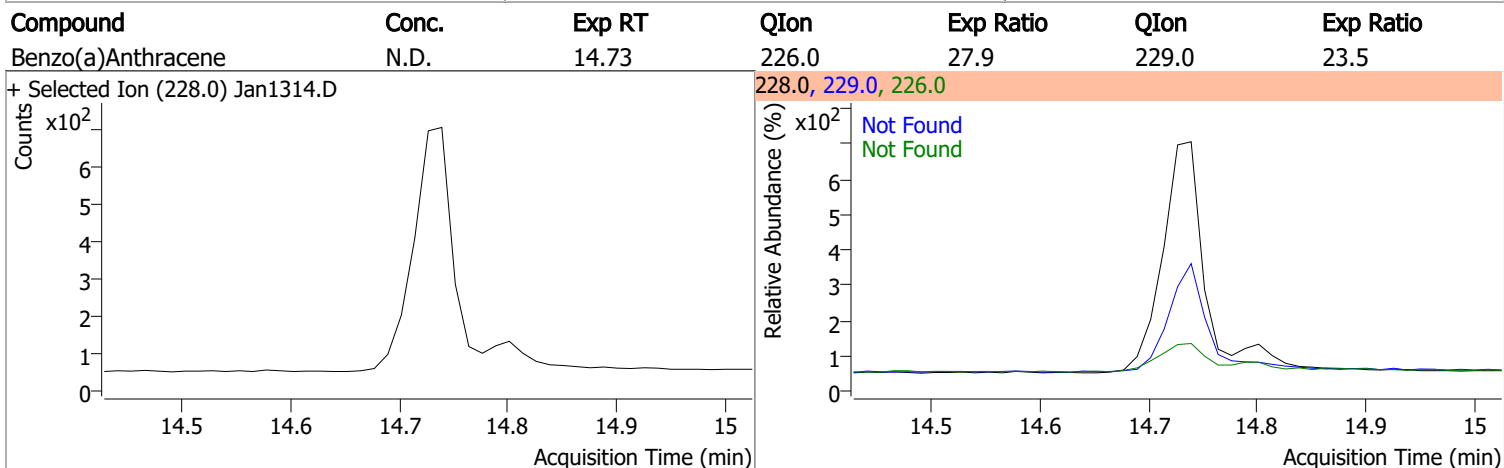


Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.76	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.82	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.6	30.8




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.24	138.0	25.2




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.32	279.0	25.9	139.0	18.3




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.58	277.0	24.5	138.0	20.0



Quantitation Results Report (QT Reviewed)

Data File	Jan1315.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/13/2022 10:45:19 PM
Sample Name	13-Jan-22_CCV_15	Instrument	GCMS
Vial	15	Multiplier	1.00
DA Method File	011222 bna SIM 1.batch.bin	Comment	SVOC-8270C-SIM-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011322 bna SIM 2.batch.bin	Last Calib Update	1/4/2022 2:09:05 PM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.509	152.0	207195	40.0000	ng/ml	-0.037
M Naphthalene-d8	5.941	136.0	380573	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.000	164.0	204579	40.0000	ng/ml	-0.013
M Phenanthrene-d10	9.780	188.0	441392	40.0000	ng/ml	-0.013
M Chrysene-d12	14.739	240.0	302477	40.0000	ng/ml	# -0.025
M Perylene-d12	18.512	264.0	248869	40.0000	ng/ml	-0.013
System Monitoring Compounds						
S Nitrobenzene-d5	5.143	82.0	9757	2.0268	ng/ml	-0.025
Spiked Amount: 5.000		Range: 19.0 - 102.0%		Recovery = 40.54%		
S 2-Fluorobiphenyl	7.252	172.0	21490	2.1100	ng/ml	-0.013
Spiked Amount: 5.000		Range: 25.0 - 94.0%		Recovery = 42.20%		
S o-Terphenyl	10.299	230.0	14142	1.7473	ng/ml	-0.025
Spiked Amount: 5.000		Range: 40.0 - 140.0%		Recovery = 34.95% *		
S Terphenyl-d14	12.263	244.0	12426	2.2200	ng/ml	# -0.025
Spiked Amount: 5.000		Range: 39.0 - 106.0%		Recovery = 44.40%		
Target Compounds						
T Naphthalene	5.953	128.0	28129	2.2011	ng/ml	95
T 2-Methylnaphthalene	6.790	141.0	15680	2.1276	ng/ml	m 96
T 1-Methylnaphthalene	6.890	141.0	15742	2.3100	ng/ml	m 94
T Acenaphthylene	7.826	152.0	25707	2.3497	ng/ml	95
T Acenaphthene	8.038	154.0	16792	2.1111	ng/ml	97
T Fluorene	8.673	166.0	19889	2.1850	ng/ml	95
T Phenanthrene	9.805	178.0	28151	2.1033	ng/ml	100
T Anthracene	9.867	178.0	24888	2.3183	ng/ml	97
T Fluoranthene	11.411	202.0	29478	1.9592	ng/ml	93
T Pyrene	11.794	202.0	32098	2.1272	ng/ml	93
T Benzo(a)Anthracene	14.701	228.0	21305	2.3407	ng/ml	99
T Chrysene	14.801	228.0	28755	2.3136	ng/ml	97
T Benzo(b)fluoranthene	17.733	252.0	19572	1.8240	ng/ml	99


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	17.795	252.0	20463	1.8733	ng/ml	97
T Benzo(a)pyrene	18.376	252.0	15431	2.0520	ng/ml	99
T Indeno(1,2,3-cd)pyrene	20.229	276.0	15453	2.0737	ng/ml	95
T Dibenzo(a,h)anthracene	20.303	278.0	16953	1.9583	ng/ml	94
T Benzo(g,h,i)perylene	20.563	276.0	22642	2.1240	ng/ml	94


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	2.0268	5.14	-0.03	9757	54.0	36.1	21.6	40.2
					128.0	33.2	21.3	39.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	2.2011	5.95	-0.03	28129	102.0	19.1	0.0	46.6
					129.0	11.1	7.6	14.1




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	2.1276	6.79	-0.01	15680 (m)	142.0	145.9	103.3	191.8
					115.0	60.6	36.8	68.3




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	2.3100	6.89	-0.01	15742 (m)	142.0	117.1	77.9	144.7
					115.0	67.9	44.4	82.5




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	2.1100	7.25	-0.01	21490	171.0	37.5	26.4	49.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthylene	2.3497	7.83	-0.01	25707	153.0	12.6	10.2	18.9






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	2.1111	8.04	-0.01	16792	153.0	116.6	80.3	149.2
					152.0	58.9	38.4	71.4






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene	2.1850	8.67	-0.01	19889	165.0	100.8	67.5	125.3
					167.0	13.5	7.9	14.6






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Phenanthrene	2.1033	9.80	-0.01	28151	176.0	15.5	10.9	20.2
					178.0	15.5	99.7	15.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Anthracene	2.3183	9.87	-0.01	24888	176.0	18.0	11.6	21.6
					178.0	18.0	108.2	18.0




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
o-Terphenyl	1.7473	10.30	-0.02	14142	229.0	70.4	46.7	86.8
					215.0	46.9	30.2	56.2




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluoranthene	1.9592	11.41	-0.02	29478	101.0	14.2	8.0	14.8




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Pyrene	2.1272	11.79	-0.02	32098	101.0	16.6	9.7	18.1



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	2.2200	12.26	-0.02	12426	122.0	19.8	9.6	17.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)Anthracene	2.3407	14.70	-0.03	21305	226.0	27.1	19.5	36.3
					229.0	23.2	16.5	30.6




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	2.3136	14.80	-0.03	28755	226.0	30.6	22.2	41.2
					229.0	20.6	15.5	28.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(b)fluoranthene	1.8240	17.73	-0.02	19572	253.0	22.0	15.8	29.4



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(k)fluoranthene	1.8733	17.79	-0.02	20463	253.0	24.5	16.1	30.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene	2.0520	18.38	-0.02	15431	253.0	24.2	16.6	30.8



Quantitation Results Report (QT Reviewed)

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Indeno(1,2,3-cd)pyrene	2.0737	20.23	-0.01	15453	138.0	27.9	17.6	32.7
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1315.D</p> </div> <div style="width: 30%;"> <p>276.0, 138.0</p> <p>Ratio = 27.9 (111.0 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.229-20.229 min, 1 scans) (**) Jan1315.D</p> <p>Lib Match Score=76.7</p> </div> </div>								
Dibenzo(a,h)anthracene	1.9583	20.30	-0.01	16953	279.0	25.3	18.1	33.6
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (278.0) Jan1315.D</p> </div> <div style="width: 30%;"> <p>278.0, 279.0, 139.0</p> <p>Ratio = 25.3 (97.7 %)</p> <p>Ratio = 23.5 (128.4 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.303-20.303 min, 1 scans) (**) Jan1315.D</p> <p>Lib Match Score=76.5</p> </div> </div>								
Benzo(g,h,i)perylene	2.1240	20.56	-0.01	22642	277.0	24.1	17.1	31.8
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1315.D</p> </div> <div style="width: 30%;"> <p>276.0, 138.0, 277.0</p> <p>Ratio = 25.7 (128.8 %)</p> <p>Ratio = 24.1 (98.3 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.563-20.563 min, 1 scans) (**) Jan1315.D</p> <p>Lib Match Score=76.4</p> </div> </div>								

Continuing Calibration Report

Batch Name \\MASSHUNTER\Org\Data\SV5975.I\sh011322\1 e8270d bna SIM\QuantResults\011322 bna SIM 2.batch.bin
Method File \\MASSHUNTER\Org\Data\SV5975.I\sh011222\1 e8270d bna SIM\011222 bna SIM 1.batch.bin
Daily CC \\MASSHUNTER\Org\Data\SV5975.I\sh011322\1 e8270d bna SIM\Jan1302.D

Level name	Injection Time	Calibration Files
7	12/28/2021 5:30:40 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2802.D
6	12/28/2021 6:03:21 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2803.D
5	12/28/2021 6:35:53 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2804.D
4	12/28/2021 7:08:33 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2805.D
3	12/28/2021 7:41:06 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2806.D
2	12/28/2021 8:13:46 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2807.D
1	12/28/2021 8:46:23 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2808.D
CCV	1/13/2022 3:43:22 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh011322\1 e8270d bna SIM\Jan1302.D <=====

ISTD Compound:	Avg Resp	Mid Resp	CC Resp	Area%	A/M
1,4-Dichlorobenzene-d4	305106	324694	199419	61.42	M
Naphthalene-d8	572584	593232	358024	60.35	M
Acenaphthene-d10	319385	333337	192587	57.78	M
Phenanthrene-d10	689765	735690	407579	55.40	M
Chrysene-d12	520451	540068	291387	53.95	M
Perylene-d12	336551	351697	222675	63.31	M

Target Compound	AvgRF/R2	CC RF	Exp. Conc	Calc. Conc	%Dev	Area%	Curve Fit
1,4-Dichlorobenzene-d4	-----ISTD-----						
Nitrobenzene-d5	0.9996	0.7777	2.00	1.69	15.43	53.69	Quadratic
Naphthalene-d8	-----ISTD-----						
Naphthalene	1.3431	1.2974	2.00	1.93	-3.41	61.26	Avg RF
2-Methylnaphthalene	0.7746	0.7495	2.00	1.94	-3.24	62.35	Avg RF
1-Methylnaphthalene	0.7163	0.7844	2.00	2.19	9.51	71.96	Avg RF
Acenaphthene-d10	-----ISTD-----						
2-Fluorobiphenyl	1.9914	1.8912	2.00	1.90	-5.03	60.62	Avg RF
Acenaphthylene	2.1392	2.3705	2.00	2.22	10.81	71.13	Avg RF
Acenaphthene	1.5553	1.5430	2.00	1.98	-0.79	61.56	Avg RF
Fluorene	1.7797	1.7657	2.00	1.98	-0.79	61.96	Avg RF
Phenanthrene-d10	-----ISTD-----						
Phenanthrene	0.9990	1.2098	2.00	1.99	0.35	57.61	Quadratic
Anthracene	0.9997	1.0158	2.00	2.09	-4.64	59.08	Quadratic
o-Terphenyl	0.7334	0.6067	2.00	1.65	-17.28	52.31	Avg RF
Fluoranthene	1.3635	1.2477	2.00	1.83	-8.49	56.78	Avg RF
Chrysene-d12	-----ISTD-----						
Pyrene	1.9954	1.8499	2.00	1.85	-7.29	54.88	Avg RF
Terphenyl-d14	0.7402	0.7296	2.00	1.97	-1.43	57.84	Avg RF
Benzo(a)Anthracene	0.9978	1.2701	2.00	2.10	-5.07	57.96	Quadratic
Chrysene	0.9966	1.7295	2.00	2.10	-5.22	58.17	Quadratic
Perylene-d12	-----ISTD-----						
Benzo(b)fluoranthene	1.7246	1.5563	2.00	1.80	-9.76	59.29	Avg RF
Benzo(k)fluoranthene	0.9999	1.7208	2.00	1.96	2.09	60.45	Quadratic
Benzo(a)pyrene	0.9996	1.2109	2.00	2.01	-0.29	63.52	Quadratic
Indeno(1,2,3-cd)pyrene	1.1977	1.2133	2.00	2.03	1.30	69.93	Avg RF
Dibenzo(a,h)anthracene	1.3915	1.3487	2.00	1.94	-3.08	66.21	Avg RF
Benzo(g,h,i)perylene	0.9993	1.7620	2.00	2.06	-2.97	64.40	Quadratic

A -- against Average; M -- against Mid Point; P -- against Previous CC in the Method;

Continuing Calibration Report

Batch Name \\MASSHUNTER\Org\Data\SV5975.I\sh011322\1 e8270d bna SIM\QuantResults\011322 bna SIM 2.batch.bin
Method File \\MASSHUNTER\Org\Data\SV5975.I\sh011222\1 e8270d bna SIM\011222 bna SIM 1.batch.bin
Daily CC \\MASSHUNTER\Org\Data\SV5975.I\sh011322\1 e8270d bna SIM\Jan1315.D

Level name	Injection Time	Calibration Files
7	12/28/2021 5:30:40 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2802.D
6	12/28/2021 6:03:21 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2803.D
5	12/28/2021 6:35:53 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2804.D
4	12/28/2021 7:08:33 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2805.D
3	12/28/2021 7:41:06 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2806.D
2	12/28/2021 8:13:46 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2807.D
1	12/28/2021 8:46:23 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh122821\1 e8270c bna SIM\Dec2808.D
CCV	1/13/2022 10:45:19 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh011322\1 e8270d bna SIM\Jan1315.D <=====

ISTD Compound:	Avg Resp	Mid Resp	CC Resp	Area%	A/M
1,4-Dichlorobenzene-d4	305106	324694	199419	61.42	M
Naphthalene-d8	572584	593232	358024	60.35	M
Acenaphthene-d10	319385	333337	192587	57.78	M
Phenanthrene-d10	689765	735690	407579	55.40	M
Chrysene-d12	520451	540068	291387	53.95	M
Perylene-d12	336551	351697	222675	63.31	M

Target Compound	AvgRF/R2	CC RF	Exp. Conc	Calc. Conc	%Dev	Area%	Curve Fit
1,4-Dichlorobenzene-d4	-----ISTD-----						
Nitrobenzene-d5	0.9996	0.7777	2.00	1.69	15.43	53.69	Quadratic
Naphthalene-d8	-----ISTD-----						
Naphthalene	1.3431	1.2974	2.00	1.93	-3.41	61.26	Avg RF
2-Methylnaphthalene	0.7746	0.7495	2.00	1.94	-3.24	62.35	Avg RF
1-Methylnaphthalene	0.7163	0.7844	2.00	2.19	9.51	71.96	Avg RF
Acenaphthene-d10	-----ISTD-----						
2-Fluorobiphenyl	1.9914	1.8912	2.00	1.90	-5.03	60.62	Avg RF
Acenaphthylene	2.1392	2.3705	2.00	2.22	10.81	71.13	Avg RF
Acenaphthene	1.5553	1.5430	2.00	1.98	-0.79	61.56	Avg RF
Fluorene	1.7797	1.7657	2.00	1.98	-0.79	61.96	Avg RF
Phenanthrene-d10	-----ISTD-----						
Phenanthrene	0.9990	1.2098	2.00	1.99	0.35	57.61	Quadratic
Anthracene	0.9997	1.0158	2.00	2.09	-4.64	59.08	Quadratic
o-Terphenyl	0.7334	0.6067	2.00	1.65	-17.28	52.31	Avg RF
Fluoranthene	1.3635	1.2477	2.00	1.83	-8.49	56.78	Avg RF
Chrysene-d12	-----ISTD-----						
Pyrene	1.9954	1.8499	2.00	1.85	-7.29	54.88	Avg RF
Terphenyl-d14	0.7402	0.7296	2.00	1.97	-1.43	57.84	Avg RF
Benzo(a)Anthracene	0.9978	1.2701	2.00	2.10	-5.07	57.96	Quadratic
Chrysene	0.9966	1.7295	2.00	2.10	-5.22	58.17	Quadratic
Perylene-d12	-----ISTD-----						
Benzo(b)fluoranthene	1.7246	1.5563	2.00	1.80	-9.76	59.29	Avg RF
Benzo(k)fluoranthene	0.9999	1.7208	2.00	1.96	2.09	60.45	Quadratic
Benzo(a)pyrene	0.9996	1.2109	2.00	2.01	-0.29	63.52	Quadratic
Indeno(1,2,3-cd)pyrene	1.1977	1.2133	2.00	2.03	1.30	69.93	Avg RF
Dibenzo(a,h)anthracene	1.3915	1.3487	2.00	1.94	-3.08	66.21	Avg RF
Benzo(g,h,i)perylene	0.9993	1.7620	2.00	2.06	-2.97	64.40	Quadratic

A -- against Average; M -- against Mid Point; P -- against Previous CC in the Method;

Audit Trail report

Batch name and path: \\MASSHUNTER\Org\Data\SV5975.I\sh011322\1 e8270d bna SIM\QuantResults\011322 bna SIM 2.batch.bin
Quant batch version: 10.0
Quant reporting version: 10.0

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdNewBatchTable	BL2000\jheine	1/13/2022 4:07:39 PM	Create new batch \\MASSHUNTER\Org\Data\SV5975.I\sh011322\1 e8270d bna SIM\011322 bna SIM 2.batch.bin			✓	
CmdImportSamplesFromWorklist	BL2000\jheine	1/13/2022 4:07:46 PM	Add samples from worklist: \\MASSHUNTER\Org\Data\SV5975.I\sh011322\1 e8270d bna SIM\Jan1302.D, \\MASSHUNTER\Org\Data\SV5975.I\sh011322\1 e8270d bna SIM\Jan1301.D			✓	
CmdSetSampleAttribute	BL2000\jheine	1/13/2022 4:07:55 PM	Set SampleType = TuneCheck for sample Jan1301.D; previous value = Sample			✓	
CmdStartMethodEditing	BL2000\jheine	1/13/2022 4:08:34 PM	Start method editing			✓	
CmdImportMethodFromBatch	BL2000\jheine	1/13/2022 4:08:35 PM	Import method from batch \\MASSHUNTER\Org\Data\SV5975.I\sh011222\1 e8270d bna SIM\011222 bna SIM 1.batch.bin			✓	
CmdApplyMethodToAllSamples	BL2000\jheine	1/13/2022 4:08:39 PM	Apply method to all samples			✓	
CmdMethodClear	BL2000\jheine	1/13/2022 4:08:39 PM	Clear method			✓	
CmdEndMethodEditing	BL2000\jheine	1/13/2022 4:08:39 PM	End method editing			✓	
CmdQuantitate	BL2000\jheine	1/13/2022 4:08:42 PM	Quantitate all compounds in all samples			✓	
CmdSetSampleAttribute	BL2000\jheine	1/13/2022 4:08:46 PM	Set SampleType = CC for sample Jan1302.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/13/2022 4:08:48 PM	Set LevelName = CCV for sample Jan1302.D; previous value =			✓	
CmdQuantitate	BL2000\jheine	1/13/2022 4:08:50 PM	Quantitate all compounds in sample Jan1302.D			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/13/2022 4:09:07 PM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1302.D, from x, y = 5.941, 708 to 6.028, 84, result = 3005; previous integration is from x, y = 5.879, 84 to 6.028, 84 and previous response = 7573.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/13/2022 4:09:08 PM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1302.D to y = 84, new integration is from x, y = 5.941, 84 to 6.028, 84 and new response = 4643; previous integration is from x, y = 5.941, 708 to 6.028, 84 and previous response = 3005.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSaveBatchTable	BL2000\jheine	1/13/2022 4:09:52 PM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011322\1 e8270d bna SIM\QuantResults\011322 bna SIM 2.batch.bin			✓	
CmdSaveBatchTable	BL2000\jheine	1/13/2022 4:10:16 PM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011322\1 e8270d bna SIM\QuantResults\011322 bna SIM 2.batch.bin			✓	
CmdManuallyIntegrate QualifierPeak	BL2000\jheine	1/13/2022 4:11:06 PM	Manually integrate qualifier 122.0 of compound Terphenyl-d14 in sample Jan1302.D, from x, y = 12.214, 66 to 12.325, 271, result = 1378; previous integration is from x, y = 12.214, 66 to 12.411, 66 and previous response = 2132.			✓	
CmdManuallyIntegrate DropBaseline	BL2000\jheine	1/13/2022 4:11:07 PM	Drop baseline for qualifier 122.0 of compound Terphenyl-d14 in sample Jan1302.D to y = 66, new integration is from x, y = 12.214, 66 to 12.325, 66 and new response = 2063; previous integration is from x, y = 12.214, 66 to 12.325, 271 and previous response = 1378.			✓	
CmdSaveBatchTable	BL2000\jheine	1/13/2022 4:11:26 PM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011322\1 e8270d bna SIM\QuantResults\011322 bna SIM 2.batch.bin			✓	
CmdSaveBatchTable	BL2000\jheine	1/13/2022 4:11:47 PM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011322\1 e8270d bna SIM\QuantResults\011322 bna SIM 2.batch.bin			✓	
CmdSaveBatchTable	BL2000\jheine	1/13/2022 4:12:37 PM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011322\1 e8270d bna SIM\QuantResults\011322 bna SIM 2.batch.bin			✓	
CmdSaveBatchTable	BL2000\jheine	1/13/2022 4:23:28 PM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011322\1 e8270d bna SIM\QuantResults\011322 bna SIM 2.batch.bin			✓	
CmdOpenBatchTable	BL2000\jheine	1/14/2022 8:26:03 AM	Open batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011322\1 e8270d bna SIM\011322 bna SIM 2.batch.bin			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdImportSamplesFromWorklist	BL2000\jheine	1/14/2022 8:27:26 AM	Add samples from worklist: \\MASSHUNTER\Org\Data\SV5975.I\sh 011322\1 e8270d bna SIM\Jan1315.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011322\1 e8270d bna SIM\Jan1314.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011322\1 e8270d bna SIM\Jan1313.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011322\1 e8270d bna SIM\Jan1312.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011322\1 e8270d bna SIM\Jan1311.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011322\1 e8270d bna SIM\Jan1310.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011322\1 e8270d bna SIM\Jan1309.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011322\1 e8270d bna SIM\Jan1308.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011322\1 e8270d bna SIM\Jan1307.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011322\1 e8270d bna SIM\Jan1306.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011322\1 e8270d bna SIM\Jan1305.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011322\1 e8270d bna SIM\Jan1304.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011322\1 e8270d bna SIM\Jan1303.D			✓	
CmdSetSampleAttribute	BL2000\jheine	1/14/2022 8:28:54 AM	Set SampleType = Calibration for sample Jan1306.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/14/2022 8:28:56 AM	Set SampleType = Blank for sample Jan1306.D; previous value = Calibration			✓	
CmdSetSampleAttribute	BL2000\jheine	1/14/2022 8:28:59 AM	Set SampleType = Matrix for sample Jan1307.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/14/2022 8:29:02 AM	Set SampleType = MatrixDup for sample Jan1308.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/14/2022 8:29:05 AM	Set SampleType = Matrix for sample Jan1312.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/14/2022 8:29:08 AM	Set SampleType = CC for sample Jan1315.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/14/2022 8:29:11 AM	Set LevelName = CCV for sample Jan1315.D; previous value =			✓	
CmdQuantitate	BL2000\jheine	1/14/2022 8:29:19 AM	Quantitate all compounds in all samples			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/14/2022 8:29:39 AM	Manually integrate compound Benzo(a)pyrene in sample Jan1303.D, from x, y = 18.351, 86 to 18.413, 155, result = -146; previous integration is from x, y = 18.463, 68 to 18.574, 70 and previous response = 1657.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/14/2022 8:29:41 AM	Snap baseline for compound Benzo(a)pyrene in sample Jan1303.D, from x = 18.351 to x = 18.413, new integration is from x, y = 18.351, 63 to 18.413, 71 and new response = 52; previous integration is from x, y = 18.351, 86 to 18.413, 155 and previous response = -146.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:29:41 AM	Drop baseline for compound Benzo(a)pyrene in sample Jan1303.D to y = 63, new integration is from x, y = 18.351, 63 to 18.413, 63 and new response = 67; previous integration is from x, y = 18.351, 63 to 18.413, 71 and previous response = 52.			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:29:44 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1303.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/14/2022 8:29:51 AM	Manually integrate compound Acenaphthene in sample Jan1303.D, from x, y = 8.026, 108 to 8.088, 65, result = 126; previous integration is from x, y = 7.971, 65 to 8.088, 65 and previous response = 1443.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:29:52 AM	Drop baseline for compound Acenaphthene in sample Jan1303.D to y = 65, new integration is from x, y = 8.026, 65 to 8.088, 65 and new response = 205; previous integration is from x, y = 8.026, 108 to 8.088, 65 and previous response = 126.			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:29:55 AM	Zero out primary peak of compound Acenaphthene in sample Jan1303.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/14/2022 8:30:03 AM	Manually integrate compound Chrysene in sample Jan1303.D, from x, y = 14.764, 130 to 14.851, 160, result = -213; previous integration is from x, y = 14.665, 55 to 14.764, 56 and previous response = 1521.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/14/2022 8:30:04 AM	Snap baseline for compound Chrysene in sample Jan1303.D, from x = 14.764 to x = 14.851, new integration is from x, y = 14.764, 109 to 14.851, 68 and new response = 81; previous integration is from x, y = 14.764, 130 to 14.851, 160 and previous response = -213.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:30:04 AM	Drop baseline for compound Chrysene in sample Jan1303.D to y = 68, new integration is from x, y = 14.764, 68 to 14.851, 68 and new response = 189; previous integration is from x, y = 14.764, 109 to 14.851, 68 and previous response = 81.			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:30:06 AM	Zero out primary peak of compound Chrysene in sample Jan1303.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/14/2022 8:31:20 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1304.D, from x, y = 5.941, 406 to 6.016, 73, result = 760; previous integration is from x, y = 5.905, 73 to 6.016, 73 and previous response = 4283.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:31:22 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1304.D to y = 73, new integration is from x, y = 5.941, 73 to 6.016, 73 and new response = 1509; previous integration is from x, y = 5.941, 406 to 6.016, 73 and previous response = 760.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/14/2022 8:31:35 AM	Manually integrate compound Acenaphthylene in sample Jan1304.D, from x, y = 7.801, 86 to 7.876, 123, result = 941; previous integration is from x, y = 8.013, 129 to 8.072, 129 and previous response = 1121.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:31:37 AM	Drop baseline for compound Acenaphthylene in sample Jan1304.D to y = 86, new integration is from x, y = 7.801, 86 to 7.876, 86 and new response = 1024; previous integration is from x, y = 7.801, 86 to 7.876, 123 and previous response = 941.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/14/2022 8:31:43 AM	Manually integrate qualifier 153.0 of compound Acenaphthylene in sample Jan1304.D from x, y = 7.813, 88 to 7.838, 98; result = 81			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:31:45 AM	Drop baseline for qualifier 153.0 of compound Acenaphthylene in sample Jan1304.D to y = 88, new integration is from x, y = 7.813, 88 to 7.838, 88 and new response = 88; previous integration is from x, y = 7.813, 88 to 7.838, 98 and previous response = 81.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/14/2022 8:32:08 AM	Manually integrate compound Acenaphthylene in sample Jan1304.D, from x, y = 7.801, 86 to 7.813, 109, result = 0; previous integration is from x, y = 7.801, 86 to 7.876, 86 and previous response = 1024.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/14/2022 8:32:13 AM	Manually integrate compound Acenaphthylene in sample Jan1304.D, from x, y = 7.838, 367 to 7.888, 257, result = -382; previous integration is from x, y = 7.801, 86 to 7.813, 109 and previous response = 0.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/14/2022 8:32:15 AM	Snap baseline for compound Acenaphthylene in sample Jan1304.D, from x = 7.838 to x = 7.888, new integration is from x, y = 7.838, 367 to 7.888, 110 and new response = -163; previous integration is from x, y = 7.838, 367 to 7.888, 257 and previous response = -382.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:32:16 AM	Drop baseline for compound Acenaphthylene in sample Jan1304.D to y = 110, new integration is from x, y = 7.838, 110 to 7.888, 110 and new response = 222; previous integration is from x, y = 7.838, 367 to 7.888, 110 and previous response = -163.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/14/2022 8:32:19 AM	Manually integrate qualifier 153.0 of compound Acenaphthylene in sample Jan1304.D, from x, y = 7.838, 181 to 7.863, 144, result = -36; previous integration is from x, y = 7.813, 88 to 7.838, 88 and previous response = 88.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/14/2022 8:32:21 AM	Snap baseline for qualifier 153.0 of compound Acenaphthylene in sample Jan1304.D from x = 7.838 to x = 7.863, new integration is from x, y = 7.838, 142 to 7.863, 94 and new response = 31; previous integration is from x, y = 7.838, 181 to 7.863, 144 and previous response = -36.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:32:23 AM	Drop baseline for qualifier 153.0 of compound Acenaphthylene in sample Jan1304.D to y = 94, new integration is from x, y = 7.838, 94 to 7.863, 94 and new response = 67; previous integration is from x, y = 7.838, 142 to 7.863, 94 and previous response = 31.			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:32:25 AM	Zero out primary peak of compound Acenaphthylene in sample Jan1304.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/14/2022 8:32:33 AM	Manually integrate compound Acenaphthene in sample Jan1304.D, from x, y = 8.025, 106 to 8.125, 85, result = 1996; previous integration is from x, y = 7.977, 83 to 8.125, 85 and previous response = 3343.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:32:34 AM	Drop baseline for compound Acenaphthene in sample Jan1304.D to y = 85, new integration is from x, y = 8.025, 85 to 8.125, 85 and new response = 2058; previous integration is from x, y = 8.025, 106 to 8.125, 85 and previous response = 1996.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegratePeak	BL2000\jheine	1/14/2022 8:33:38 AM	Manually integrate compound Benzo(a)pyrene in sample Jan1305.D, from x, y = 18.363, 162 to 18.462, 216, result = 97; previous integration is from x, y = 18.464, 116 to 18.573, 120 and previous response = 1625.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/14/2022 8:33:39 AM	Snap baseline for compound Benzo(a)pyrene in sample Jan1305.D, from x = 18.363 to x = 18.462, new integration is from x, y = 18.363, 120 to 18.462, 112 and new response = 532; previous integration is from x, y = 18.363, 162 to 18.462, 216 and previous response = 97.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:33:40 AM	Drop baseline for compound Benzo(a)pyrene in sample Jan1305.D to y = 112, new integration is from x, y = 18.363, 112 to 18.462, 112 and new response = 555; previous integration is from x, y = 18.363, 120 to 18.462, 112 and previous response = 532.			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:33:41 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1305.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/14/2022 8:33:46 AM	Manually integrate compound Acenaphthene in sample Jan1305.D, from x, y = 8.025, 102 to 8.147, 69, result = 206; previous integration is from x, y = 7.978, 69 to 8.147, 69 and previous response = 1443.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:33:48 AM	Drop baseline for compound Acenaphthene in sample Jan1305.D to y = 69, new integration is from x, y = 8.025, 69 to 8.147, 69 and new response = 325; previous integration is from x, y = 8.025, 102 to 8.147, 69 and previous response = 206.			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:33:50 AM	Zero out primary peak of compound Acenaphthene in sample Jan1305.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/14/2022 8:33:55 AM	Manually integrate compound Anthracene in sample Jan1305.D, from x, y = 9.842, 195 to 9.916, 293, result = -185; previous integration is from x, y = 9.758, 88 to 9.842, 88 and previous response = 1617.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/14/2022 8:33:57 AM	Snap baseline for compound Anthracene in sample Jan1305.D, from x = 9.842 to x = 9.916, new integration is from x, y = 9.842, 107 to 9.916, 97 and new response = 448; previous integration is from x, y = 9.842, 195 to 9.916, 293 and previous response = -185.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrate DropBaseline	BL2000\jheine	1/14/2022 8:33:58 AM	Drop baseline for compound Anthracene in sample Jan1305.D to y = 97, new integration is from x, y = 9.842, 97 to 9.916, 97 and new response = 470; previous integration is from x, y = 9.842, 107 to 9.916, 97 and previous response = 448.			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:33:59 AM	Zero out primary peak of compound Anthracene in sample Jan1305.D			✓	
CmdManuallyIntegrate QualifierPeak	BL2000\jheine	1/14/2022 8:34:06 AM	Manually integrate qualifier 229.0 of compound Chrysene in sample Jan1305.D, from x, y = 14.776, 106 to 14.901, 73, result = 326; previous integration is from x, y = 14.975, 73 to 15.398, 77 and previous response = 388.			✓	
CmdManuallyIntegrate DropBaseline	BL2000\jheine	1/14/2022 8:34:08 AM	Drop baseline for qualifier 229.0 of compound Chrysene in sample Jan1305.D to y = 73, new integration is from x, y = 14.776, 73 to 14.901, 73 and new response = 450; previous integration is from x, y = 14.776, 106 to 14.901, 73 and previous response = 326.			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:34:11 AM	Zero out primary peak of compound Chrysene in sample Jan1305.D			✓	
CmdManuallyIntegrate QualifierPeak	BL2000\jheine	1/14/2022 8:34:16 AM	Manually integrate qualifier 229.0 of compound Benzo(a)Anthracene in sample Jan1305.D, from x, y = 14.664, 71 to 14.776, 106, result = 783; previous integration is from x, y = 14.664, 71 to 14.901, 73 and previous response = 1351.			✓	
CmdManuallyIntegrate DropBaseline	BL2000\jheine	1/14/2022 8:34:18 AM	Drop baseline for qualifier 229.0 of compound Benzo(a)Anthracene in sample Jan1305.D to y = 71, new integration is from x, y = 14.664, 71 to 14.776, 71 and new response = 900; previous integration is from x, y = 14.664, 71 to 14.776, 106 and previous response = 783.			✓	
CmdManuallyIntegrate QualifierPeak	BL2000\jheine	1/14/2022 8:34:23 AM	Manually integrate qualifier 226.0 of compound Benzo(a)Anthracene in sample Jan1305.D, from x, y = 14.652, 66 to 14.764, 84, result = 397; previous integration is from x, y = 14.764, 70 to 14.950, 71 and previous response = 520.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:34:24 AM	Drop baseline for qualifier 226.0 of compound Benzo(a)Anthracene in sample Jan1305.D to y = 66, new integration is from x, y = 14.652, 66 to 14.764, 66 and new response = 456; previous integration is from x, y = 14.652, 66 to 14.764, 84 and previous response = 397.			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:34:28 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1305.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:34:30 AM	Zero out primary peak of compound Indeno(1,2,3-cd)pyrene in sample Jan1305.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:34:32 AM	Zero out primary peak of compound Phenanthrene in sample Jan1305.D			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/14/2022 8:34:37 AM	Manually integrate qualifier 253.0 of compound Benzo(b)fluoranthene in sample Jan1305.D from x, y = 17.708, 91 to 17.783, 99; result = 174			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:34:38 AM	Drop baseline for qualifier 253.0 of compound Benzo(b)fluoranthene in sample Jan1305.D to y = 91, new integration is from x, y = 17.708, 91 to 17.783, 91 and new response = 191; previous integration is from x, y = 17.708, 91 to 17.783, 99 and previous response = 174.			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:34:39 AM	Zero out primary peak of compound Benzo(b)fluoranthene in sample Jan1305.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:34:42 AM	Zero out primary peak of compound Benzo(g,h,i)perylene in sample Jan1305.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/14/2022 8:35:20 AM	Manually integrate compound Fluorene in sample Jan1306.D, from x, y = 8.649, 71 to 8.711, 72, result = 100; previous integration is from x, y = 8.948, 68 to 9.072, 68 and previous response = 13109.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/14/2022 8:35:21 AM	Snap baseline for compound Fluorene in sample Jan1306.D, from x = 8.649 to x = 8.711, new integration is from x, y = 8.649, 67 to 8.711, 72 and new response = 107; previous integration is from x, y = 8.649, 71 to 8.711, 72 and previous response = 100.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:35:22 AM	Drop baseline for compound Fluorene in sample Jan1306.D to y = 67, new integration is from x, y = 8.649, 67 to 8.711, 67 and new response = 116; previous integration is from x, y = 8.649, 67 to 8.711, 72 and previous response = 107.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:35:24 AM	Zero out primary peak of compound Fluorene in sample Jan1306.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:35:27 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1306.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/14/2022 8:35:32 AM	Manually integrate compound Acenaphthene in sample Jan1306.D, from x, y = 8.025, 98 to 8.150, 71, result = 116; previous integration is from x, y = 7.963, 71 to 8.150, 71 and previous response = 1523.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:35:34 AM	Drop baseline for compound Acenaphthene in sample Jan1306.D to y = 71, new integration is from x, y = 8.025, 71 to 8.150, 71 and new response = 217; previous integration is from x, y = 8.025, 98 to 8.150, 71 and previous response = 116.			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:35:35 AM	Zero out primary peak of compound Acenaphthene in sample Jan1306.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/14/2022 8:35:40 AM	Manually integrate compound Chrysene in sample Jan1306.D, from x, y = 14.776, 205 to 14.876, 56, result = -153; previous integration is from x, y = 14.664, 56 to 14.876, 56 and previous response = 2011.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:35:41 AM	Drop baseline for compound Chrysene in sample Jan1306.D to y = 56, new integration is from x, y = 14.776, 56 to 14.876, 56 and new response = 291; previous integration is from x, y = 14.776, 205 to 14.876, 56 and previous response = -153.			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:35:43 AM	Zero out primary peak of compound Chrysene in sample Jan1306.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/14/2022 8:35:48 AM	Manually integrate compound Benzo(a)Anthracene in sample Jan1306.D, from x, y = 14.664, 56 to 14.776, 93, result = 1595; previous integration is from x, y = 14.664, 56 to 14.876, 56 and previous response = 2011.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:35:49 AM	Drop baseline for compound Benzo(a)Anthracene in sample Jan1306.D to y = 56, new integration is from x, y = 14.664, 56 to 14.776, 56 and new response = 1720; previous integration is from x, y = 14.664, 56 to 14.776, 93 and previous response = 1595.			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:35:51 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1306.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/14/2022 8:36:05 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1307.D, from x, y = 5.941, 842 to 6.040, 87, result = 6991; previous integration is from x, y = 5.903, 87 to 6.040, 87 and previous response = 12433.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:36:06 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1307.D to y = 87, new integration is from x, y = 5.941, 87 to 6.040, 87 and new response = 9254; previous integration is from x, y = 5.941, 842 to 6.040, 87 and previous response = 6991.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/14/2022 8:36:16 AM	Manually integrate compound 1-Methylnaphthalene in sample Jan1307.D, from x, y = 6.865, 111 to 6.965, 3176, result = 18160; previous integration is from x, y = 6.865, 111 to 7.052, 125 and previous response = 28519.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:36:18 AM	Drop baseline for compound 1-Methylnaphthalene in sample Jan1307.D to y = 111, new integration is from x, y = 6.865, 111 to 6.965, 111 and new response = 27344; previous integration is from x, y = 6.865, 111 to 6.965, 3176 and previous response = 18160.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/14/2022 8:36:21 AM	Set UserAnnotation = CO for compound 1-Methylnaphthalene in sample Jan1307.D; previous value =			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/14/2022 8:37:20 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1308.D, from x, y = 5.941, 732 to 6.041, 81, result = 5587; previous integration is from x, y = 5.903, 81 to 6.041, 81 and previous response = 10696.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:37:21 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1308.D to y = 81, new integration is from x, y = 5.941, 81 to 6.041, 81 and new response = 7536; previous integration is from x, y = 5.941, 732 to 6.041, 81 and previous response = 5587.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/14/2022 8:37:30 AM	Manually integrate compound 2-Methylnaphthalene in sample Jan1308.D, from x, y = 6.765, 2229 to 6.877, 2804, result = 8012; previous integration is from x, y = 6.628, 95 to 7.052, 95 and previous response = 49372.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/14/2022 8:37:31 AM	Snap baseline for compound 2-Methylnaphthalene in sample Jan1308.D, from x = 6.765 to x = 6.877, new integration is from x, y = 6.765, 131 to 6.877, 408 and new response = 23167; previous integration is from x, y = 6.765, 2229 to 6.877, 2804 and previous response = 8012.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:37:32 AM	Drop baseline for compound 2-Methylnaphthalene in sample Jan1308.D to y = 131, new integration is from x, y = 6.765, 131 to 6.877, 131 and new response = 24101; previous integration is from x, y = 6.765, 131 to 6.877, 408 and previous response = 23167.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/14/2022 8:37:43 AM	Set UserAnnotation = CO for compound 2-Methylnaphthalene in sample Jan1308.D; previous value =			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/14/2022 8:37:50 AM	Manually integrate compound 1-Methylnaphthalene in sample Jan1308.D, from x, y = 6.877, 1727 to 6.965, 2589, result = 11890; previous integration is from x, y = 6.628, 95 to 7.052, 95 and previous response = 49372.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/14/2022 8:37:51 AM	Snap baseline for compound 1-Methylnaphthalene in sample Jan1308.D, from x = 6.877 to x = 6.965, new integration is from x, y = 6.877, 408 to 6.965, 385 and new response = 21131; previous integration is from x, y = 6.877, 1727 to 6.965, 2589 and previous response = 11890.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:37:52 AM	Drop baseline for compound 1-Methylnaphthalene in sample Jan1308.D to y = 385, new integration is from x, y = 6.877, 385 to 6.965, 385 and new response = 21191; previous integration is from x, y = 6.877, 408 to 6.965, 385 and previous response = 21131.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/14/2022 8:37:55 AM	Set UserAnnotation = CO for compound 1-Methylnaphthalene in sample Jan1308.D; previous value =			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/14/2022 8:38:03 AM	Manually integrate qualifier153.0 of compound Acenaphthylene in sample Jan1308.D from x, y = 7.801, 1578 to 7.863, 5765; result = -6948			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/14/2022 8:38:05 AM	Snap baseline for qualifier 153.0 of compound Acenaphthylene in sample Jan1308.D from x = 7.801 to x = 7.863, new integration is from x, y = 7.801, 73 to 7.863, 310 and new response = 6061; previous integration is from x, y = 7.801, 1578 to 7.863, 5765 and previous response = -6948.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:38:05 AM	Drop baseline for qualifier 153.0 of compound Acenaphthylene in sample Jan1308.D to y = 73, new integration is from x, y = 7.801, 73 to 7.863, 73 and new response = 6504; previous integration is from x, y = 7.801, 73 to 7.863, 310 and previous response = 6061.			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:38:52 AM	Zero out primary peak of compound Fluorene in sample Jan1309.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:38:57 AM	Zero out primary peak of compound 1-Methylnaphthalene in sample Jan1309.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/14/2022 8:39:04 AM	Manually integrate compound Benzo(a)pyrene in sample Jan1309.D, from x, y = 18.363, 104 to 18.413, 190, result = -171; previous integration is from x, y = 18.467, 80 to 18.561, 82 and previous response = 1670.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/14/2022 8:39:05 AM	Snap baseline for compound Benzo(a)pyrene in sample Jan1309.D, from x = 18.363 to x = 18.413, new integration is from x, y = 18.363, 71 to 18.413, 76 and new response = 46; previous integration is from x, y = 18.363, 104 to 18.413, 190 and previous response = -171.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:39:06 AM	Drop baseline for compound Benzo(a)pyrene in sample Jan1309.D to y = 71, new integration is from x, y = 18.363, 71 to 18.413, 71 and new response = 54; previous integration is from x, y = 18.363, 71 to 18.413, 76 and previous response = 46.			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:39:07 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1309.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:39:13 AM	Zero out primary peak of compound 2-Methylnaphthalene in sample Jan1309.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:39:21 AM	Zero out primary peak of compound Acenaphthene in sample Jan1309.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegratePeak	BL2000\jheine	1/14/2022 8:39:26 AM	Manually integrate compound Chrysene in sample Jan1309.D, from x, y = 14.776, 108 to 14.876, 122, result = -105; previous integration is from x, y = 14.664, 59 to 14.826, 59 and previous response = 1831.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/14/2022 8:39:28 AM	Snap baseline for compound Chrysene in sample Jan1309.D, from x = 14.776 to x = 14.876, new integration is from x, y = 14.776, 108 to 14.876, 68 and new response = 57; previous integration is from x, y = 14.776, 108 to 14.876, 122 and previous response = -105.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:39:29 AM	Drop baseline for compound Chrysene in sample Jan1309.D to y = 68, new integration is from x, y = 14.776, 68 to 14.876, 68 and new response = 177; previous integration is from x, y = 14.776, 108 to 14.876, 68 and previous response = 57.			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:39:30 AM	Zero out primary peak of compound Chrysene in sample Jan1309.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:39:44 AM	Zero out primary peak of compound Naphthalene in sample Jan1309.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/14/2022 8:40:07 AM	Manually integrate compound Fluorene in sample Jan1310.D, from x, y = 8.649, 138 to 8.711, 138, result = 201; previous integration is from x, y = 8.948, 155 to 9.110, 155 and previous response = 9874.			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:40:09 AM	Zero out primary peak of compound Fluorene in sample Jan1310.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/14/2022 8:40:17 AM	Manually integrate compound Acenaphthene in sample Jan1310.D, from x, y = 8.026, 172 to 8.050, 204, result = 181; previous integration is from x, y = 7.978, 177 to 8.163, 177 and previous response = 2195.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:40:18 AM	Drop baseline for compound Acenaphthene in sample Jan1310.D to y = 172, new integration is from x, y = 8.026, 172 to 8.050, 172 and new response = 205; previous integration is from x, y = 8.026, 172 to 8.050, 204 and previous response = 181.			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:40:20 AM	Zero out primary peak of compound Acenaphthene in sample Jan1310.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:40:30 AM	Zero out primary peak of compound 1-Methylnaphthalene in sample Jan1310.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:40:33 AM	Zero out primary peak of compound 2-Methylnaphthalene in sample Jan1310.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:40:35 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1310.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:40:37 AM	Zero out primary peak of compound Naphthalene in sample Jan1310.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:40:38 AM	Zero out primary peak of compound Chrysene in sample Jan1310.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/14/2022 8:40:58 AM	Manually integrate compound Fluorene in sample Jan1311.D, from x, y = 8.649, 122 to 8.698, 214, result = -161; previous integration is from x, y = 8.925, 82 to 9.060, 82 and previous response = 9591.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/14/2022 8:40:59 AM	Snap baseline for compound Fluorene in sample Jan1311.D, from x = 8.649 to x = 8.698, new integration is from x, y = 8.649, 78 to 8.698, 88 and new response = 92; previous integration is from x, y = 8.649, 122 to 8.698, 214 and previous response = -161.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:41:00 AM	Drop baseline for compound Fluorene in sample Jan1311.D to y = 78, new integration is from x, y = 8.649, 78 to 8.698, 78 and new response = 107; previous integration is from x, y = 8.649, 78 to 8.698, 88 and previous response = 92.			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:41:01 AM	Zero out primary peak of compound Fluorene in sample Jan1311.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:41:04 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1311.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:41:06 AM	Zero out primary peak of compound Acenaphthene in sample Jan1311.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:41:07 AM	Zero out primary peak of compound Chrysene in sample Jan1311.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:41:09 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1311.D			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/14/2022 8:41:25 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1312.D, from x, y = 5.941, 783 to 6.041, 99, result = 5185; previous integration is from x, y = 5.903, 96 to 6.041, 99 and previous response = 11046.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:41:26 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1312.D to y = 99, new integration is from x, y = 5.941, 99 to 6.041, 99 and new response = 7237; previous integration is from x, y = 5.941, 783 to 6.041, 99 and previous response = 5185.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/14/2022 8:41:38 AM	Manually integrate qualifier 153.0 of compound Acenaphthylene in sample Jan1312.D from x, y = 7.814, 2820 to 7.876, 5303; result = -8291			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/14/2022 8:41:39 AM	Snap baseline for qualifier 153.0 of compound Acenaphthylene in sample Jan1312.D from x = 7.814 to x = 7.876, new integration is from x, y = 7.814, 215 to 7.876, 254 and new response = 6015; previous integration is from x, y = 7.814, 2820 to 7.876, 5303 and previous response = -8291.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:41:40 AM	Drop baseline for qualifier 153.0 of compound Acenaphthylene in sample Jan1312.D to y = 215, new integration is from x, y = 7.814, 215 to 7.876, 215 and new response = 6087; previous integration is from x, y = 7.814, 215 to 7.876, 254 and previous response = 6015.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/14/2022 8:42:01 AM	Manually integrate qualifier 122.0 of compound Terphenyl-d14 in sample Jan1312.D, from x, y = 12.214, 72 to 12.312, 695, result = 3610; previous integration is from x, y = 12.214, 72 to 12.386, 72 and previous response = 5602.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:42:02 AM	Drop baseline for qualifier 122.0 of compound Terphenyl-d14 in sample Jan1312.D to y = 72, new integration is from x, y = 12.214, 72 to 12.312, 72 and new response = 5440; previous integration is from x, y = 12.214, 72 to 12.312, 695 and previous response = 3610.			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:42:55 AM	Zero out primary peak of compound Fluorene in sample Jan1313.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:42:58 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1313.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/14/2022 8:43:04 AM	Manually integrate compound Acenaphthene in sample Jan1313.D, from x, y = 8.025, 100 to 8.088, 68, result = 99; previous integration is from x, y = 7.963, 68 to 8.088, 68 and previous response = 1385.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:43:06 AM	Drop baseline for compound Acenaphthene in sample Jan1313.D to y = 68, new integration is from x, y = 8.025, 68 to 8.088, 68 and new response = 158; previous integration is from x, y = 8.025, 100 to 8.088, 68 and previous response = 99.			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:43:07 AM	Zero out primary peak of compound Acenaphthene in sample Jan1313.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:43:09 AM	Zero out primary peak of compound Chrysene in sample Jan1313.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/14/2022 8:43:49 AM	Manually integrate compound Fluorene in sample Jan1314.D, from x, y = 8.636, 65 to 8.698, 67, result = 120; previous integration is from x, y = 8.936, 67 to 9.060, 67 and previous response = 8980.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:43:50 AM	Drop baseline for compound Fluorene in sample Jan1314.D to y = 65, new integration is from x, y = 8.636, 65 to 8.698, 65 and new response = 124; previous integration is from x, y = 8.636, 65 to 8.698, 67 and previous response = 120.			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:43:52 AM	Zero out primary peak of compound Fluorene in sample Jan1314.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:43:56 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1314.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/14/2022 8:44:00 AM	Manually integrate compound Acenaphthene in sample Jan1314.D, from x, y = 8.025, 106 to 8.075, 70, result = 77; previous integration is from x, y = 7.976, 70 to 8.075, 70 and previous response = 1323.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:44:01 AM	Drop baseline for compound Acenaphthene in sample Jan1314.D to y = 70, new integration is from x, y = 8.025, 70 to 8.075, 70 and new response = 130; previous integration is from x, y = 8.025, 106 to 8.075, 70 and previous response = 77.			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:44:02 AM	Zero out primary peak of compound Acenaphthene in sample Jan1314.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/14/2022 8:44:05 AM	Zero out primary peak of compound Chrysene in sample Jan1314.D			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/14/2022 8:44:36 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1315.D, from x, y = 5.941, 883 to 6.041, 71, result = 2927; previous integration is from x, y = 5.903, 71 to 6.041, 71 and previous response = 8582.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:44:38 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1315.D to y = 71, new integration is from x, y = 5.941, 71 to 6.041, 71 and new response = 5359; previous integration is from x, y = 5.941, 883 to 6.041, 71 and previous response = 2927.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateSplit	BL2000\jheine	1/14/2022 8:44:43 AM	Split peak for compound 2-Methylnaphthalene in sample Jan1315.D and keep left peak, new integration is from x, y = 6.752, 83.1283333333333 to 6.865, 83.1283333333333 and new response = 15680, previous integration is from x, y = 6.752, 83 to 7.052, 83 and previous response = 32341.			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	1/14/2022 8:44:51 AM	Split peak for compound 1-Methylnaphthalene in sample Jan1315.D and keep right peak, new integration is from x, y = 6.865, 83.1283333333333 to 7.052, 83.1283333333333 and new response = 16660, previous integration is from x, y = 6.752, 83 to 7.052, 83 and previous response = 32341.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/14/2022 8:44:56 AM	Manually integrate compound 1-Methylnaphthalene in sample Jan1315.D, from x, y = 6.865, 83 to 6.965, 1961, result = 10114; previous integration is from x, y = 6.865, 83 to 7.052, 83 and previous response = 16660.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:44:58 AM	Drop baseline for compound 1-Methylnaphthalene in sample Jan1315.D to y = 83, new integration is from x, y = 6.865, 83 to 6.965, 83 and new response = 15742; previous integration is from x, y = 6.865, 83 to 6.965, 1961 and previous response = 10114.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/14/2022 8:45:10 AM	Manually integrate qualifier 153.0 of compound Acenaphthylene in sample Jan1315.D from x, y = 7.814, 1136 to 7.863, 3561; result = -3432			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/14/2022 8:45:11 AM	Snap baseline for qualifier 153.0 of compound Acenaphthylene in sample Jan1315.D from x = 7.814 to x = 7.863, new integration is from x, y = 7.814, 122 to 7.863, 214 and new response = 3090; previous integration is from x, y = 7.814, 1136 to 7.863, 3561 and previous response = -3432.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/14/2022 8:45:12 AM	Drop baseline for qualifier 153.0 of compound Acenaphthylene in sample Jan1315.D to y = 122, new integration is from x, y = 7.814, 122 to 7.863, 122 and new response = 3228; previous integration is from x, y = 7.814, 122 to 7.863, 214 and previous response = 3090.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSaveBatchTable	BL2000\jheine	1/14/2022 8:45:48 AM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011322\1 e8270d bna SIM\QuantResults\011322 bna SIM 2.batch.bin			✓	
CmdSaveBatchTable	BL2000\jheine	1/14/2022 8:46:20 AM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011322\1 e8270d bna SIM\QuantResults\011322 bna SIM 2.batch.bin			✓	
CmdSetSampleAttribute	BL2000\jheine	1/14/2022 8:47:37 AM	Set SampleApproved = True for sample Jan1301.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/14/2022 8:47:39 AM	Set SampleApproved = True for sample Jan1302.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/14/2022 8:47:40 AM	Set SampleApproved = True for sample Jan1303.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/14/2022 8:47:43 AM	Set SampleApproved = True for sample Jan1307.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/14/2022 8:47:45 AM	Set SampleApproved = True for sample Jan1306.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/14/2022 8:47:47 AM	Set SampleApproved = True for sample Jan1308.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/14/2022 8:47:48 AM	Set SampleApproved = True for sample Jan1309.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/14/2022 8:47:49 AM	Set SampleApproved = True for sample Jan1310.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/14/2022 8:47:51 AM	Set SampleApproved = True for sample Jan1311.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/14/2022 8:47:53 AM	Set SampleApproved = True for sample Jan1312.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/14/2022 8:47:54 AM	Set SampleApproved = True for sample Jan1313.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/14/2022 8:47:56 AM	Set SampleApproved = True for sample Jan1314.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/14/2022 8:47:57 AM	Set SampleApproved = True for sample Jan1315.D; previous value = False			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSaveBatchTable	BL2000\jheine	1/14/2022 8:48:00 AM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011322\1 e8270d bna SIM\QuantResults\011322 bna SIM 2.batch.bin			✓	
CmdOpenBatchTable	BL2000\jheine	2/3/2022 5:02:02 PM	Open batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011322\1 e8270d bna SIM\011322 bna SIM 2.batch.bin			✓	
CmdQuantitate	BL2000\jheine	2/3/2022 5:02:51 PM	Quantitate all compounds in all samples			✓	
CmdSaveBatchTable	BL2000\jheine	2/3/2022 5:02:54 PM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011322\1 e8270d bna SIM\QuantResults\011322 bna SIM 2.batch.bin			✓	
GenerateReport	BL2000\jheine	2/3/2022 5:08:39 PM	Generates report - Method: D:\Org\reports\GCMSEMI Report Templates\Tests_for_LevelIV\Env_Qua ntResults_wGraphics+Chromatogram. m, Output Path: \\MASSHUNTER\Org\Data\SV5975.I\sh 011322\1 e8270d bna SIM\QuantReports\			✓	
GenerateReport	BL2000\jheine	2/3/2022 5:14:39 PM	Generates report - Method: D:\Org\reports\GCMSEMI Report Templates\Tests_for_LevelIV\Env_Qua ntResults_wGraphics+Chromatogram. m, Output Path: \\MASSHUNTER\Org\Data\SV5975.I\sh 011322\1 e8270d bna SIM\QuantReports\			✓	

Energy Laboratories Inc

ANALYTICAL RUN Summary

04-Feb-22

Run ID SV5975.I_220114A

Run Start Date: 1/14/2022
Analyst: John P. Heine
Ical:
Column ID: ZB-SemiVolatiles
Comments:

Std ID	Std Name	Std Amount	Std Units	Samp Amount	Samp Units	SampType	Expiration Date
dcmsvoc13	DCM						11/17/2022
sv100210	BNA 2nd source 200ug/mL	2	ul	198	ul	ICV	1/15/2022
sv100506	BNA low 50 ug/mL	8	ul	192	ul	CCV	3/31/2022
sv100703	BNA Internals 2000 ug/mL	2	ul	100	ul	SAMP	5/31/2022
sv83311	DFTPP 1000 ug/mL	50	ul	50	ul	TUNE	10/31/2022

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14980592	Jan1410_D_TU	SVOC-8270-DF	TUNE	V5975.I\sh0114221	14/2022 4:18:0	1	R373230		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
127, % of mass 198	A	%	58.8	58.8		100	0	0	0	0.01	0	59%	40	60	0%	
197, % of mass 198	A	%	0	0		100	0	0	0	0.01	0	0%	0	0.99	0%	
198, Base Peak	A	%	100	100		100	0	0	0	0.01	0	100%	100	100	0%	
199, % of mass 198	A	%	6.8	6.8		100	0	0	0	0.01	0	7%	5	9	0%	
275, % of mass 198	A	%	27.6	27.6		100	0	0	0	0.01	0	28%	10	30	0%	
365, % of mass 198	A	%	3.2	3.2		100	0	0	0	0.01	0	3%	1	99.99	0%	
441, % of mass 443	A	%	94.3	94.3		100	0	0	0	0.01	0	94%	0.01	150	0%	
442, % of mass 198	A	%	64.8	64.8		100	0	0	0	0.01	0	65%	40	100	0%	
443, % of mass 442	A	%	19.2	19.2		100	0	0	0	0.01	0	19%	17	23	0%	
51, % of mass 198	A	%	48.4	48.4		100	0	0	0	0.01	0	48%	30	60	0%	
68, % of mass 69	A	%	0	0		100	0	0	0	0.01	0	0%	0	1.99	0%	
70, % of mass 69	A	%	0.4	0.4		100	0	0	0	0.01	0	0%	0	1.99	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14980593	14-Jan-22_CAL_	SVOC-8270-W-	ICAL	V5975.I\sh0114221/14/2022	4:42:2	1	R373230		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	9.50102	9.50102		10	0	0	0.0206	0.1	10	95%	20	120	0%	
2-Methylnaphthalene	A	ug/L	9.7276	9.7276		10	0	0	0.0176	0.1	10	97%	20	120	0%	
Acenaphthene	A	ug/L	9.5126	9.5126		10	0	0	0.0317	0.1	10	95%	20	120	0%	
Acenaphthylene	A	ug/L	10.69239	10.69239		10	0	0	0.025	0.1	10	107%	20	120	0%	
Anthracene	A	ug/L	10.01775	10.01775		10	0	0	0.0283	0.1	10	100%	20	120	0%	
Benzo(a)anthracene	A	ug/L	10.02184	10.02184		10	0	0	0.0272	0.1	10	100%	20	120	0%	
Benzo(a)pyrene	A	ug/L	10.0209	10.0209		10	0	0	0.0347	0.1	10	100%	20	120	0%	
Benzo(b)fluoranthene	A	ug/L	11.07554	11.07554		10	0	0	0.0226	0.1	10	111%	20	120	0%	
Benzo(g,h,i)perylene	A	ug/L	10.02903	10.02903		10	0	0	0.0267	0.1	10	100%	20	120	0%	
Benzo(k)fluoranthene	A	ug/L	9.97888	9.97888		10	0	0	0.0295	0.1	10	100%	20	120	0%	
Chrysene	A	ug/L	9.53889	9.53889		10	0	0	0.0458	0.1	10	95%	20	120	0%	
Dibenzo(a,h)anthracene	A	ug/L	10.94419	10.94419		10	0	0	0.0367	0.1	10	109%	20	120	0%	
Fluoranthene	A	ug/L	10.18625	10.18625		10	0	0	0.0233	0.1	10	102%	20	120	0%	
Fluorene	A	ug/L	9.68209	9.68209		10	0	0	0.0225	0.1	10	97%	20	120	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	10.00516	10.00516		10	0	0	0.0491	0.1	10	100%	20	120	0%	
Naphthalene	A	ug/L	10.1018	10.1018		10	0	0	0.029	0.1	10	101%	20	120	0%	
Phenanthrene	A	ug/L	10.01682	10.01682		10	0	0	0.0295	0.1	10	100%	20	120	0%	
Pyrene	A	ug/L	10.17961	10.17961		10	0	0	0.0239	0.1	10	102%	20	120	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
2-Fluorobiphenyl	S	ug/L	10.12421	10.12421		10	0	0	0.0444	0.1	10	101%	20	120	0%	
Nitrobenzene-d5	S	ug/L	9.99758	9.99758		10	0	0	0.0523	0.1	10	100%	20	120	0%	
Terphenyl-d14	S	ug/L	10.0104	10.0104		10	0	0	0.0563	0.1	10	100%	20	120	0%	
o-Terphenyl	X	ug/L	9.52874	9.52874		10	0	0	0.0654	0.1	10	95%	20	120	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14980594	14-Jan-22_CAL_	SVOC-8270-W-	ICAL	V5975.I\sh0114221/14/2022	5:14:4	1	R373230		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14980594	14-Jan-22_CAL_	SVOC-8270-W-	ICAL	V5975.I\sh0114221/14/2022	5:14:4	1	R373230		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	4.58115	4.58115		5	0	0	0.0206	0.1	10	92%	20	120	0%	
2-Methylnaphthalene	A	ug/L	4.65936	4.65936		5	0	0	0.0176	0.1	10	93%	20	120	0%	
Acenaphthene	A	ug/L	4.70812	4.70812		5	0	0	0.0317	0.1	10	94%	20	120	0%	
Acenaphthylene	A	ug/L	4.93138	4.93138		5	0	0	0.025	0.1	10	99%	20	120	0%	
Anthracene	A	ug/L	4.94657	4.94657		5	0	0	0.0283	0.1	10	99%	20	120	0%	
Benzo(a)anthracene	A	ug/L	4.93171	4.93171		5	0	0	0.0272	0.1	10	99%	20	120	0%	
Benzo(a)pyrene	A	ug/L	4.93889	4.93889		5	0	0	0.0347	0.1	10	99%	20	120	0%	
Benzo(b)fluoranthene	A	ug/L	5.0532	5.0532		5	0	0	0.0226	0.1	10	101%	20	120	0%	
Benzo(g,h,i)perylene	A	ug/L	4.91764	4.91764		5	0	0	0.0267	0.1	10	98%	20	120	0%	
Benzo(k)fluoranthene	A	ug/L	5.05302	5.05302		5	0	0	0.0295	0.1	10	101%	20	120	0%	
Chrysene	A	ug/L	4.61514	4.61514		5	0	0	0.0458	0.1	10	92%	20	120	0%	
Dibenzo(a,h)anthracene	A	ug/L	5.03779	5.03779		5	0	0	0.0367	0.1	10	101%	20	120	0%	
Fluoranthene	A	ug/L	4.87191	4.87191		5	0	0	0.0233	0.1	10	97%	20	120	0%	
Fluorene	A	ug/L	4.68279	4.68279		5	0	0	0.0225	0.1	10	94%	20	120	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	4.97155	4.97155		5	0	0	0.0491	0.1	10	99%	20	120	0%	
Naphthalene	A	ug/L	4.80463	4.80463		5	0	0	0.029	0.1	10	96%	20	120	0%	
Phenanthrene	A	ug/L	4.94768	4.94768		5	0	0	0.0295	0.1	10	99%	20	120	0%	
Pyrene	A	ug/L	4.6369	4.6369		5	0	0	0.0239	0.1	10	93%	20	120	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
2-Fluorobiphenyl	S	ug/L	4.81281	4.81281		5	0	0	0.0444	0.1	10	96%	20	120	0%	
Nitrobenzene-d5	S	ug/L	5.00273	5.00273		5	0	0	0.0523	0.1	10	100%	20	120	0%	
Terphenyl-d14	S	ug/L	4.96273	4.96273		5	0	0	0.0563	0.1	10	99%	20	120	0%	
o-Terphenyl	X	ug/L	4.62338	4.62338		5	0	0	0.0654	0.1	10	92%	20	120	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14980595	14-Jan-22_CAL_	SVOC-8270-W-	ICAL	V5975.I\sh0114221/14/2022	5:47:1	1	R373230		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14980595	14-Jan-22_CAL_	SVOC-8270-W-	ICAL	V5975.I\sh0114221/14/2022	5:47:1	1	R373230		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	1.85144	1.85144		2	0	0	0.0206	0.1	10	93%	20	120	0%	
2-Methylnaphthalene	A	ug/L	1.98647	1.98647		2	0	0	0.0176	0.1	10	99%	20	120	0%	
Acenaphthene	A	ug/L	1.91541	1.91541		2	0	0	0.0317	0.1	10	96%	20	120	0%	
Acenaphthylene	A	ug/L	1.8998	1.8998		2	0	0	0.025	0.1	10	95%	20	120	0%	
Anthracene	A	ug/L	2.03964	2.03964		2	0	0	0.0283	0.1	10	102%	20	120	0%	
Benzo(a)anthracene	A	ug/L	2.0469	2.0469		2	0	0	0.0272	0.1	10	102%	20	120	0%	
Benzo(a)pyrene	A	ug/L	2.01732	2.01732		2	0	0	0.0347	0.1	10	101%	20	120	0%	
Benzo(b)fluoranthene	A	ug/L	2.02203	2.02203		2	0	0	0.0226	0.1	10	101%	20	120	0%	
Benzo(g,h,i)perylene	A	ug/L	2.02675	2.02675		2	0	0	0.0267	0.1	10	101%	20	120	0%	
Benzo(k)fluoranthene	A	ug/L	2.00453	2.00453		2	0	0	0.0295	0.1	10	100%	20	120	0%	
Chrysene	A	ug/L	1.90834	1.90834		2	0	0	0.0458	0.1	10	95%	20	120	0%	
Dibenzo(a,h)anthracene	A	ug/L	1.82121	1.82121		2	0	0	0.0367	0.1	10	91%	20	120	0%	
Fluoranthene	A	ug/L	1.9135	1.9135		2	0	0	0.0233	0.1	10	96%	20	120	0%	
Fluorene	A	ug/L	1.92587	1.92587		2	0	0	0.0225	0.1	10	96%	20	120	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	2.05636	2.05636		2	0	0	0.0491	0.1	10	103%	20	120	0%	
Naphthalene	A	ug/L	1.89994	1.89994		2	0	0	0.029	0.1	10	95%	20	120	0%	
Phenanthrene	A	ug/L	2.05092	2.05092		2	0	0	0.0295	0.1	10	103%	20	120	0%	
Pyrene	A	ug/L	1.98327	1.98327		2	0	0	0.0239	0.1	10	99%	20	120	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
2-Fluorobiphenyl	S	ug/L	1.91595	1.91595		2	0	0	0.0444	0.1	10	96%	20	120	0%	
Nitrobenzene-d5	S	ug/L	2.01735	2.01735		2	0	0	0.0523	0.1	10	101%	20	120	0%	
Terphenyl-d14	S	ug/L	2.05065	2.05065		2	0	0	0.0563	0.1	10	103%	20	120	0%	
o-Terphenyl	X	ug/L	1.95744	1.95744		2	0	0	0.0654	0.1	10	98%	20	120	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14980596	14-Jan-22_CAL_	SVOC-8270-W-	ICAL	V5975.I\sh0114221/14/2022	6:19:4	1	R373230		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14980596	14-Jan-22_CAL_	SVOC-8270-W-	ICAL	V5975.I\sh0114221/14/2022	6:19:4	1	R373230		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0.94538	0.94538		1	0	0	0.0206	0.1	10	95%	20	120	0%	
2-Methylnaphthalene	A	ug/L	0.97552	0.97552		1	0	0	0.0176	0.1	10	98%	20	120	0%	
Acenaphthene	A	ug/L	0.95606	0.95606		1	0	0	0.0317	0.1	10	96%	20	120	0%	
Acenaphthylene	A	ug/L	0.91149	0.91149		1	0	0	0.025	0.1	10	91%	20	120	0%	
Anthracene	A	ug/L	0.9893	0.9893		1	0	0	0.0283	0.1	10	99%	20	120	0%	
Benzo(a)anthracene	A	ug/L	1.0017	1.0017		1	0	0	0.0272	0.1	10	100%	20	120	0%	
Benzo(a)pyrene	A	ug/L	1.02157	1.02157		1	0	0	0.0347	0.1	10	102%	20	120	0%	
Benzo(b)fluoranthene	A	ug/L	0.93601	0.93601		1	0	0	0.0226	0.1	10	94%	20	120	0%	
Benzo(g,h,i)perylene	A	ug/L	1.02674	1.02674		1	0	0	0.0267	0.1	10	103%	20	120	0%	
Benzo(k)fluoranthene	A	ug/L	0.95303	0.95303		1	0	0	0.0295	0.1	10	95%	20	120	0%	
Chrysene	A	ug/L	0.96628	0.96628		1	0	0	0.0458	0.1	10	97%	20	120	0%	
Dibenzo(a,h)anthracene	A	ug/L	0.93988	0.93988		1	0	0	0.0367	0.1	10	94%	20	120	0%	
Fluoranthene	A	ug/L	0.94418	0.94418		1	0	0	0.0233	0.1	10	94%	20	120	0%	
Fluorene	A	ug/L	0.95818	0.95818		1	0	0	0.0225	0.1	10	96%	20	120	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	0.98883	0.98883		1	0	0	0.0491	0.1	10	99%	20	120	0%	
Naphthalene	A	ug/L	0.97384	0.97384		1	0	0	0.029	0.1	10	97%	20	120	0%	
Phenanthrene	A	ug/L	0.98235	0.98235		1	0	0	0.0295	0.1	10	98%	20	120	0%	
Pyrene	A	ug/L	0.97339	0.97339		1	0	0	0.0239	0.1	10	97%	20	120	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
2-Fluorobiphenyl	S	ug/L	0.9422	0.9422		1	0	0	0.0444	0.1	10	94%	20	120	0%	
Nitrobenzene-d5	S	ug/L	0.99567	0.99567		1	0	0	0.0523	0.1	10	100%	20	120	0%	
Terphenyl-d14	S	ug/L	0.97722	0.97722		1	0	0	0.0563	0.1	10	98%	20	120	0%	
o-Terphenyl	X	ug/L	0.9433	0.9433		1	0	0	0.0654	0.1	10	94%	20	120	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14980597	14-Jan-22_CAL_	SVOC-8270-W-	ICAL	V5975.I\sh0114221/14/2022	6:52:1	1	R373230		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14980597	14-Jan-22_CAL_	SVOC-8270-W-	ICAL	V5975.I\sh0114221/14/2022	6:52:1	1	R373230		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0.51073	0.51073		0.5	0	0	0.0206	0.1	10	102%	20	120	0%	
2-Methylnaphthalene	A	ug/L	0.50435	0.50435		0.5	0	0	0.0176	0.1	10	101%	20	120	0%	
Acenaphthene	A	ug/L	0.47743	0.47743		0.5	0	0	0.0317	0.1	10	95%	20	120	0%	
Acenaphthylene	A	ug/L	0.488	0.488		0.5	0	0	0.025	0.1	10	98%	20	120	0%	
Anthracene	A	ug/L	0.5092	0.5092		0.5	0	0	0.0283	0.1	10	102%	20	120	0%	
Benzo(a)anthracene	A	ug/L	0.50701	0.50701		0.5	0	0	0.0272	0.1	10	101%	20	120	0%	
Benzo(a)pyrene	A	ug/L	0.5068	0.5068		0.5	0	0	0.0347	0.1	10	101%	20	120	0%	
Benzo(b)fluoranthene	A	ug/L	0.45703	0.45703		0.5	0	0	0.0226	0.1	10	91%	20	120	0%	
Benzo(g,h,i)perylene	A	ug/L	0.49816	0.49816		0.5	0	0	0.0267	0.1	10	100%	20	120	0%	
Benzo(k)fluoranthene	A	ug/L	0.48829	0.48829		0.5	0	0	0.0295	0.1	10	98%	20	120	0%	
Chrysene	A	ug/L	0.4993	0.4993		0.5	0	0	0.0458	0.1	10	100%	20	120	0%	
Dibenzo(a,h)anthracene	A	ug/L	0.46522	0.46522		0.5	0	0	0.0367	0.1	10	93%	20	120	0%	
Fluoranthene	A	ug/L	0.48488	0.48488		0.5	0	0	0.0233	0.1	10	97%	20	120	0%	
Fluorene	A	ug/L	0.49977	0.49977		0.5	0	0	0.0225	0.1	10	100%	20	120	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	0.47636	0.47636		0.5	0	0	0.0491	0.1	10	95%	20	120	0%	
Naphthalene	A	ug/L	0.5004	0.5004		0.5	0	0	0.029	0.1	10	100%	20	120	0%	
Phenanthrene	A	ug/L	0.50591	0.50591		0.5	0	0	0.0295	0.1	10	101%	20	120	0%	
Pyrene	A	ug/L	0.49726	0.49726		0.5	0	0	0.0239	0.1	10	99%	20	120	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
2-Fluorobiphenyl	S	ug/L	0.47818	0.47818		0.5	0	0	0.0444	0.1	10	96%	20	120	0%	
Nitrobenzene-d5	S	ug/L	0.48956	0.48956		0.5	0	0	0.0523	0.1	10	98%	20	120	0%	
Terphenyl-d14	S	ug/L	0.50103	0.50103		0.5	0	0	0.0563	0.1	10	100%	20	120	0%	
o-Terphenyl	X	ug/L	0.49604	0.49604		0.5	0	0	0.0654	0.1	10	99%	20	120	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14980598	14-Jan-22_CAL_	SVOC-8270-W-	ICAL	V5975.I\sh0114221/14/2022	7:24:3	1	R373230		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14980598	14-Jan-22_CAL_	SVOC-8270-W-	ICAL	V5975.I\sh0114221/14/2022	7:24:3	1	R373230		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0.21178	0.21178		0.2	0	0	0.0206	0.1	10	106%	20	120	0%	
2-Methylnaphthalene	A	ug/L	0.20359	0.20359		0.2	0	0	0.0176	0.1	10	102%	20	120	0%	
Acenaphthene	A	ug/L	0.2086	0.2086		0.2	0	0	0.0317	0.1	10	104%	20	120	0%	
Acenaphthylene	A	ug/L	0.20134	0.20134		0.2	0	0	0.025	0.1	10	101%	20	120	0%	
Anthracene	A	ug/L	0.19961	0.19961		0.2	0	0	0.0283	0.1	10	100%	20	120	0%	
Benzo(a)anthracene	A	ug/L	0.18894	0.18894		0.2	0	0	0.0272	0.1	10	94%	20	120	0%	
Benzo(a)pyrene	A	ug/L	0.19971	0.19971		0.2	0	0	0.0347	0.1	10	100%	20	120	0%	
Benzo(b)fluoranthene	A	ug/L	0.18252	0.18252		0.2	0	0	0.0226	0.1	10	91%	20	120	0%	
Benzo(g,h,i)perylene	A	ug/L	0.21092	0.21092		0.2	0	0	0.0267	0.1	10	105%	20	120	0%	
Benzo(k)fluoranthene	A	ug/L	0.23186	0.23186		0.2	0	0	0.0295	0.1	10	116%	20	120	0%	
Chrysene	A	ug/L	0.22675	0.22675		0.2	0	0	0.0458	0.1	10	113%	20	120	0%	
Dibenzo(a,h)anthracene	A	ug/L	0.20746	0.20746		0.2	0	0	0.0367	0.1	10	104%	20	120	0%	
Fluoranthene	A	ug/L	0.20335	0.20335		0.2	0	0	0.0233	0.1	10	102%	20	120	0%	
Fluorene	A	ug/L	0.20495	0.20495		0.2	0	0	0.0225	0.1	10	102%	20	120	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	0.19626	0.19626		0.2	0	0	0.0491	0.1	10	98%	20	120	0%	
Naphthalene	A	ug/L	0.19966	0.19966		0.2	0	0	0.029	0.1	10	100%	20	120	0%	
Phenanthrene	A	ug/L	0.19492	0.19492		0.2	0	0	0.0295	0.1	10	97%	20	120	0%	
Pyrene	A	ug/L	0.20164	0.20164		0.2	0	0	0.0239	0.1	10	101%	20	120	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
2-Fluorobiphenyl	S	ug/L	0.20887	0.20887		0.2	0	0	0.0444	0.1	10	104%	20	120	0%	
Nitrobenzene-d5	S	ug/L	0.18791	0.18791		0.2	0	0	0.0523	0.1	10	94%	20	120	0%	
Terphenyl-d14	S	ug/L	0.19562	0.19562		0.2	0	0	0.0563	0.1	10	98%	20	120	0%	
o-Terphenyl	X	ug/L	0.20674	0.20674		0.2	0	0	0.0654	0.1	10	103%	20	120	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14980599	14-Jan-22_CAL_	SVOC-8270-W-	ICAL	V5975.I\sh0114221/14/2022	7:57:0	1	R373230		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14980599	14-Jan-22_CAL_	SVOC-8270-W-	ICAL	V5975.I\sh0114221/14/2022	7:57:0	1	R373230		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0.11822	0.11822		0.1	0	0	0.0206	0.1	10	118%	20	120	0%	
2-Methylnaphthalene	A	ug/L	0.11	0.11		0.1	0	0	0.0176	0.1	10	110%	20	120	0%	
Acenaphthene	A	ug/L	0.11955	0.11955		0.1	0	0	0.0317	0.1	10	120%	20	120	0%	
Acenaphthylene	A	ug/L	0.11004	0.11004		0.1	0	0	0.025	0.1	10	110%	20	120	0%	
Anthracene	A	ug/L	0.09833	0.09833		0.1	0	0	0.0283	0.1	10	98%	20	120	0%	
Benzo(a)anthracene	A	ug/L	0.10275	0.10275		0.1	0	0	0.0272	0.1	10	103%	20	120	0%	
Benzo(a)pyrene	A	ug/L	0.09676	0.09676		0.1	0	0	0.0347	0.1	10	97%	20	120	0%	
Benzo(b)fluoranthene	A	ug/L	0.11081	0.11081		0.1	0	0	0.0226	0.1	10	111%	20	120	0%	
Benzo(g,h,i)perylene	A	ug/L	0.09224	0.09224		0.1	0	0	0.0267	0.1	10	92%	20	120	0%	
Benzo(k)fluoranthene	A	ug/L	0.09003	0.09003		0.1	0	0	0.0295	0.1	10	90%	20	120	0%	
Chrysene	A	ug/L	0.10703	0.10703		0.1	0	0	0.0458	0.1	10	107%	20	120	0%	
Dibenzo(a,h)anthracene	A	ug/L	0.10798	0.10798		0.1	0	0	0.0367	0.1	10	108%	20	120	0%	
Fluoranthene	A	ug/L	0.11196	0.11196		0.1	0	0	0.0233	0.1	10	112%	20	120	0%	
Fluorene	A	ug/L	0.11498	0.11498		0.1	0	0	0.0225	0.1	10	115%	20	120	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	0.10541	0.10541		0.1	0	0	0.0491	0.1	10	105%	20	120	0%	
Naphthalene	A	ug/L	0.1106	0.1106		0.1	0	0	0.029	0.1	10	111%	20	120	0%	
Phenanthrene	A	ug/L	0.10145	0.10145		0.1	0	0	0.0295	0.1	10	101%	20	120	0%	
Pyrene	A	ug/L	0.10869	0.10869		0.1	0	0	0.0239	0.1	10	109%	20	120	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
2-Fluorobiphenyl	S	ug/L	0.11241	0.11241		0.1	0	0	0.0444	0.1	10	112%	20	120	0%	
Nitrobenzene-d5	S	ug/L	0.10768	0.10768		0.1	0	0	0.0523	0.1	10	108%	20	120	0%	
Terphenyl-d14	S	ug/L	0.10237	0.10237		0.1	0	0	0.0563	0.1	10	102%	20	120	0%	
o-Terphenyl	X	ug/L	0.11747	0.11747		0.1	0	0	0.0654	0.1	10	117%	20	120	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14980600	14-Jan-22_CCV	SVOC-8270-W-	ICV	V5975.I\sh0114221/14/2022	8:29:2	1	R373230		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14980600	14-Jan-22_CC	SVOC-8270-W-	ICV	V5975.I\sh0114221/14/2022	8:29:2	1	R373230		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	2.04721	2.04721		2	0	0	0.0206	0.1	10	102%	80	120	0%	
2-Methylnaphthalene	A	ug/L	2.36322	2.36322		2	0	0	0.0176	0.1	10	118%	80	120	0%	
Acenaphthene	A	ug/L	2.26243	2.26243		2	0	0	0.0317	0.1	10	113%	80	120	0%	
Acenaphthylene	A	ug/L	2.05883	2.05883		2	0	0	0.025	0.1	10	103%	80	120	0%	
Anthracene	A	ug/L	2.20817	2.20817		2	0	0	0.0283	0.1	10	110%	80	120	0%	
Benzo(a)anthracene	A	ug/L	2.33474	2.33474		2	0	0	0.0272	0.1	10	117%	80	120	0%	
Benzo(a)pyrene	A	ug/L	2.14743	2.14743		2	0	0	0.0347	0.1	10	107%	80	120	0%	
Benzo(b)fluoranthene	A	ug/L	2.28767	2.28767		2	0	0	0.0226	0.1	10	114%	80	120	0%	
Benzo(g,h,i)perylene	A	ug/L	2.32809	2.32809		2	0	0	0.0267	0.1	10	116%	80	120	0%	
Benzo(k)fluoranthene	A	ug/L	2.1338	2.1338		2	0	0	0.0295	0.1	10	107%	80	120	0%	
Chrysene	A	ug/L	2.16915	2.16915		2	0	0	0.0458	0.1	10	108%	80	120	0%	
Dibenzo(a,h)anthracene	A	ug/L	2.05215	2.05215		2	0	0	0.0367	0.1	10	103%	80	120	0%	
Fluoranthene	A	ug/L	2.10934	2.10934		2	0	0	0.0233	0.1	10	105%	80	120	0%	
Fluorene	A	ug/L	2.18671	2.18671		2	0	0	0.0225	0.1	10	109%	80	120	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	2.1963	2.1963		2	0	0	0.0491	0.1	10	110%	80	120	0%	
Naphthalene	A	ug/L	2.19434	2.19434		2	0	0	0.029	0.1	10	110%	80	120	0%	
Phenanthrene	A	ug/L	2.25334	2.25334		2	0	0	0.0295	0.1	10	113%	80	120	0%	
Pyrene	A	ug/L	2.12371	2.12371		2	0	0	0.0239	0.1	10	106%	80	120	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
2-Fluorobiphenyl	S	ug/L	1.98767	1.98767		2	0	0	0.0444	0.1	10	99%	80	120	0%	
Nitrobenzene-d5	S	ug/L	2.05804	2.05804		2	0	0	0.0523	0.1	10	103%	80	120	0%	
o-Terphenyl	S	ug/L	2.09304	2.09304		2	0	0	0.0654	0.1	10	105%	80	120	0%	
Terphenyl-d14	S	ug/L	1.929	1.929		2	0	0	0.0563	0.1	10	96%	80	120	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14980601	14-Jan-22_ISTB	SVOC-8270-W-	SAMP	V5975.I\sh0114221/14/2022	9:01:5	1	R373230		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q



Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14980601	14-Jan-22_ISTB	SVOC-8270-W-	SAMP	V5975.I\sh0114221/14/2022	9:01:5	1	R373230		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0206	0.1	10	0%	0	0	0%	
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0176	0.1	10	0%	0	0	0%	
Acenaphthene	A	ug/L	0	0		0	0	0	0.0317	0.1	10	0%	0	0	0%	
Acenaphthylene	A	ug/L	0	0		0	0	0	0.025	0.1	10	0%	0	0	0%	
Anthracene	A	ug/L	0	0		0	0	0	0.0283	0.1	10	0%	0	0	0%	
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.0272	0.1	10	0%	0	0	0%	
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.0347	0.1	10	0%	0	0	0%	
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.0226	0.1	10	0%	0	0	0%	
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.0267	0.1	10	0%	0	0	0%	
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.0295	0.1	10	0%	0	0	0%	
Chrysene	A	ug/L	0	0		0	0	0	0.0458	0.1	10	0%	0	0	0%	
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.0367	0.1	10	0%	0	0	0%	
Fluoranthene	A	ug/L	0	0		0	0	0	0.0233	0.1	10	0%	0	0	0%	
Fluorene	A	ug/L	0	0		0	0	0	0.0225	0.1	10	0%	0	0	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.0491	0.1	10	0%	0	0	0%	
Naphthalene	A	ug/L	0	0		0	0	0	0.029	0.1	10	0%	0	0	0%	
Phenanthrene	A	ug/L	0	0		0	0	0	0.0295	0.1	10	0%	0	0	0%	
Pyrene	A	ug/L	0	0		0	0	0	0.0239	0.1	10	0%	0	0	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
2-Fluorobiphenyl	S	ug/L	0	0		5	0	0	0.0444	0.1	10	0%	25	94	0%	S
Nitrobenzene-d5	S	ug/L	0	0		5	0	0	0.0523	0.1	10	0%	19	102	0%	S
Terphenyl-d14	S	ug/L	0	0		5	0	0	0.0563	0.1	10	0%	39	106	0%	S
o-Terphenyl	X	ug/L	0	0		200	0	0	0.0654	0.1	10	0%	40	140	0%	S

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14980602	MB-162910-162	SVOC-8270-W-	MBLK	V5975.I\sh0114221/14/2022	9:34:1	1	162910	12/14/2021	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

File Name	Sample Name	Line No.	Test Code	Multiplier	Divisor	Method Name
Jan1401.d	14-Jan-22_TUNE_1	1		1	1	548Tune.M
Jan1402.d	ICAL-4-162632	2	SVOC-548-W-DW	1	1	5975Endothall.M
Jan1403.d	14-Jan-22_ISTBLK_3	3	SVOC-548-W-DW	1	1	5975Endothall.M
Jan1404.d	MB-162839	4	SVOC-548-W-DW	1	1	5975Endothall.M
Jan1405.d	LCS-162839	5	SVOC-548-W-DW	1	1	5975Endothall.M
Jan1406.d	B22010259-001B	6	SVOC-548-W-DW	1	1	5975Endothall.M
Jan1407.d	B22010259-001BMS	7	SVOC-548-W-DW	1	1	5975Endothall.M
Jan1408.d	B22010259-001BMSD	8	SVOC-548-W-DW	1	1	5975Endothall.M
Jan1409.d	B22010309-002C	9	SVOC-548-W-DW	1	1	5975Endothall.M
Jan1410.d	14-Jan-22_TUNE_10	10		1	1	5975Tune.M
Jan1411.d	14-Jan-22_CAL_7	11	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1412.d	14-Jan-22_CAL_6	12	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1413.d	14-Jan-22_CAL_5	13	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1414.d	14-Jan-22_CAL_4	14	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1415.d	14-Jan-22_CAL_3	15	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1416.d	14-Jan-22_CAL_2	16	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1417.d	14-Jan-22_CAL_1	17	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1418.d	14-Jan-22_CCV_18	18	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1419.d	14-Jan-22_ISTBLK_19	19	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1420.d	MB-162910-162494-162167	20	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1421.d	MB-162910-162494-162167	21	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Jan1422.d	LCS-162910-162494-162167	22	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Jan1423.d	B21120800-003D	23	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Jan1424.d	B21120800-003DMS	24	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Jan1425.d	B21120800-003DMSD	25	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Jan1426.d	B21120838-006D	26	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1427.d	B21120838-006D	27	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M
Jan1428.d	B21120838-007D	28	SVOC-8270-W-LLPAH	1	1	5975BNASIM.M
Jan1429.d	B21120838-007D	29	SVOC-8270-W-LLPAH	20	1	5975BNASIM.M









Tune Evaluation Report

Data Path: \\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIMJan1410.D
 Acq on: 1/14/2022 4:18:41 PM
 Operator: LIMS import
 Sample: 14-Jan-22_TUNE_10
 Inst Name: GCMS
 ALS Vial: 1
 Method: \\MASSHUNTER\Org\Data\SV5975.I\Methods\DFTPP5975625.m




Target Mass	Rel. To Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Pass/Fail
51	198	30	60	48.4	113144	Pass
68	69	0	2	0.0	0	Pass
70	69	0	2	0.4	742	Pass
127	198	40	60	58.8	137600	Pass
197	198	0	1	0.0	0	Pass
198	198	100	100	100.0	233856	Pass
199	198	5	9	6.8	15867	Pass
275	198	10	30	27.6	64440	Pass
365	198	1	100	3.2	7575	Pass
441	443	1E-10	150	94.3	27376	Pass
442	198	40	100	64.8	151424	Pass
443	442	17	23	19.2	29024	Pass
69	69	100	100	100.0	177856	Pass

Tune Evaluation Report



Tune Evaluation Report


+ Scan (rt: 8.181-8.220 min, 28 scans) Jan1410.D 4,4'-DDE




Compound Name	Expected RT	Observed RT	TIC Area	Breakdown %	Pass/Fail
4,4'-DDT	8.800	8.707	3193264	0.3	Pass
4,4'-DDD	8.500	8.406	9082		
4,4'-DDE	8.200	0.000	0		

Tune Evaluation Report

+ Scan (rt: 6.403 min) Jan1410.D Pentachlorophenol



+ Scan (rt: 7.930 min) Jan1410.D Benzidine




Compound Name	Expected RT	Observed RT	Tailing Factor	PGF	Pass/Fail
Pentachlorophenol	6.800	6.403	0.4	4.1	Pass
Benzidine	8.400	7.930	0.2	2.7	Pass

Calibration Report

Batch Path	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\QuantResults\011422 bna SIM 2.batch.bin	Analyst Name	BL2000\jheine
Analysis Time	2/4/2022 3:29 PM	Reporter Name	BL2000\jheine
Report Time	2/4/2022 3:30:35 PM	Batch State	Processed
Last Calib Update	1/17/2022 8:49 AM	Quant Report Version	10.0
Quant Batch Version	10.0		

Nitrobenzene-d5 %RSE =




Calibration STD Path	Cal Type	Level	Enabled	Resp.	Exp. Conc	Resp. Factor	Level RSD
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1417.D	Calibration	1	x	285	0.1000	0.6985	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1416.D	Calibration	2	x	517	0.2000	0.6299	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1415.D	Calibration	3	x	1431	0.5000	0.6832	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1414.D	Calibration	4	x	3242	1.0000	0.7196	
\\MASSHUNTER\Org\Data\SV5975.I\sh010421\1 e8270c bna SIM\Jan0402.D	CC	CCV	x	16927	2.0000	0.8426	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1418.D	QC	ICV	x	7442	2.0000	0.7896	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1413.D	Calibration	5	x	6699	2.0000	0.7724	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1412.D	Calibration	6	x	20380	5.0000	0.8862	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1411.D	Calibration	7	x	49501	10.0000	1.0843	

Calibration Report

Batch Path	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\QuantResults\011422 bna SIM 2.batch.bin	Analyst Name	BL2000\jheine
Analysis Time	2/4/2022 3:29 PM	Reporter Name	BL2000\jheine
Report Time	2/4/2022 3:30:40 PM	Batch State	Processed
Last Calib Update	1/17/2022 8:49 AM	Quant Report Version	10.0
Quant Batch Version	10.0		

Naphthalene %RSE = 5.2




Calibration STD Path	Cal Type	Level	Enabled	Resp.	Exp. Conc	Resp. Factor	Level RSD
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1417.D	Calibration	1	x	1112	0.1000	1.5305	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1416.D	Calibration	2	x	2073	0.2000	1.3815	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1415.D	Calibration	3	x	5189	0.5000	1.3850	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1414.D	Calibration	4	x	11085	1.0000	1.3477	
\\MASSHUNTER\Org\Data\SV5975.I\sh010421\1 e8270c bna SIM\Jan0402.D	CC	CCV	x	43467	2.0000	1.1266	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1418.D	QC	ICV	x	25149	2.0000	1.5183	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1413.D	Calibration	5	x	21057	2.0000	1.3146	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1412.D	Calibration	6	x	54816	5.0000	1.3298	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1411.D	Calibration	7	x	113952	10.0000	1.3980	

Calibration Report

Batch Path	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\QuantResults\011422 bna SIM 2.batch.bin		
Analysis Time	2/4/2022 3:29 PM	Analyst Name	BL2000\jheine
Report Time	2/4/2022 3:30:41 PM	Reporter Name	BL2000\jheine
Last Calib Update	1/17/2022 8:49 AM	Batch State	Processed
Quant Batch Version	10.0	Quant Report Version	10.0

2-Methylnaphthalene %RSE = 5.2

2-Methylnaphthalene - 7 Levels, 7 Levels Used, 7 Points, 7 Points Used, 1 QCs




Calibration STD Path	Cal Type	Level	Enabled	Resp.	Exp. Conc	Resp. Factor	Level RSD
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1417.D	Calibration	1	x	617	0.1000	0.8496	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1416.D	Calibration	2	x	1180	0.2000	0.7863	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1415.D	Calibration	3	x	2919	0.5000	0.7791	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1414.D	Calibration	4	x	6198	1.0000	0.7535	
\\MASSHUNTER\Org\Data\SV5975.I\sh010421\1 e8270c bna SIM\Jan0402.D	CC	CCV	x	26546	2.0000	0.6880	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1418.D	QC	ICV	x	15117	2.0000	0.9127	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1413.D	Calibration	5	x	12288	2.0000	0.7672	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1412.D	Calibration	6	x	29670	5.0000	0.7198	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1411.D	Calibration	7	x	61246	10.0000	0.7514	

Calibration Report

Batch Path	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\QuantResults\011422 bna SIM 2.batch.bin		
Analysis Time	2/4/2022 3:29 PM	Analyst Name	BL2000\jheine
Report Time	2/4/2022 3:30:41 PM	Reporter Name	BL2000\jheine
Last Calib Update	1/17/2022 8:49 AM	Batch State	Processed
Quant Batch Version	10.0	Quant Report Version	10.0

1-Methylnaphthalene %RSE = 9.6




Calibration STD Path	Cal Type	Level	Enabled	Resp.	Exp. Conc	Resp. Factor	Level RSD
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1417.D	Calibration	1	x	700	0.1000	0.9631	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1416.D	Calibration	2	x	1294	0.2000	0.8626	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1415.D	Calibration	3	x	3118	0.5000	0.8321	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1414.D	Calibration	4	x	6335	1.0000	0.7701	
\\MASSHUNTER\Org\Data\SV5975.I\sh010421\1 e8270c bna SIM\Jan0402.D	CC	CCV	x	26180	2.0000	0.6786	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1418.D	QC	ICV	x	13812	2.0000	0.8339	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1413.D	Calibration	5	x	12079	2.0000	0.7541	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1412.D	Calibration	6	x	30767	5.0000	0.7464	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1411.D	Calibration	7	x	63090	10.0000	0.7740	

Calibration Report

Batch Path	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\QuantResults\011422 bna SIM 2.batch.bin		
Analysis Time	2/4/2022 3:29 PM	Analyst Name	BL2000\jheine
Report Time	2/4/2022 3:30:41 PM	Reporter Name	BL2000\jheine
Last Calib Update	1/17/2022 8:49 AM	Batch State	Processed
Quant Batch Version	10.0	Quant Report Version	10.0

2-Fluorobiphenyl %RSE =

2-Fluorobiphenyl - 7 Levels, 7 Levels Used, 7 Points, 7 Points Used, 1 QCs




Calibration STD Path	Cal Type	Level	Enabled	Resp.	Exp. Conc	Resp. Factor	Level RSD
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1417.D	Calibration	1	x	861	0.1000	2.1613	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1416.D	Calibration	2	x	1673	0.2000	2.0080	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1415.D	Calibration	3	x	3783	0.5000	1.8388	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1414.D	Calibration	4	x	8063	1.0000	1.8115	
\\MASSHUNTER\Org\Data\SV5975.I\sh010421\1 e8270c bna SIM\Jan0402.D	CC	CCV	x	41814	2.0000	2.0259	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1418.D	QC	ICV	x	17342	2.0000	1.9108	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1413.D	Calibration	5	x	15824	2.0000	1.8419	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1412.D	Calibration	6	x	40190	5.0000	1.8507	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1411.D	Calibration	7	x	85326	10.0000	1.9466	

Calibration Report

Batch Path	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\QuantResults\011422 bna SIM 2.batch.bin	Analyst Name	BL2000\jheine
Analysis Time	2/4/2022 3:29 PM	Reporter Name	BL2000\jheine
Report Time	2/4/2022 3:30:41 PM	Batch State	Processed
Last Calib Update	1/17/2022 8:49 AM	Quant Report Version	10.0
Quant Batch Version	10.0		

Acenaphthylene %RSE = 6.6




Calibration STD Path	Cal Type	Level	Enabled	Resp.	Exp. Conc	Resp. Factor	Level RSD
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1417.D	Calibration	1	x	1074	0.1000	2.6975	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1416.D	Calibration	2	x	2056	0.2000	2.4678	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1415.D	Calibration	3	x	4922	0.5000	2.3925	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1414.D	Calibration	4	x	9945	1.0000	2.2344	
\\MASSHUNTER\Org\Data\SV5975.I\sh010421\1 e8270c bna SIM\Jan0402.D	CC	CCV	x	45154	2.0000	2.1877	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1418.D	QC	ICV	x	22902	2.0000	2.5235	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1413.D	Calibration	5	x	20005	2.0000	2.3285	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1412.D	Calibration	6	x	52503	5.0000	2.4177	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1411.D	Calibration	7	x	114894	10.0000	2.6211	

Calibration Report

Batch Path	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\QuantResults\011422 bna SIM 2.batch.bin		
Analysis Time	2/4/2022 3:29 PM	Analyst Name	BL2000\jheine
Report Time	2/4/2022 3:30:41 PM	Reporter Name	BL2000\jheine
Last Calib Update	1/17/2022 8:49 AM	Batch State	Processed
Quant Batch Version	10.0	Quant Report Version	10.0

Acenaphthene %RSE = 9.3




Calibration STD Path	Cal Type	Level	Enabled	Resp.	Exp. Conc	Resp. Factor	Level RSD
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1417.D	Calibration	1	x	747	0.1000	1.8746	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1416.D	Calibration	2	x	1362	0.2000	1.6355	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1415.D	Calibration	3	x	3080	0.5000	1.4973	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1414.D	Calibration	4	x	6673	1.0000	1.4992	
\\MASSHUNTER\Org\Data\SV5975.I\sh010421\1 e8270c bna SIM\Jan0402.D	CC	CCV	x	30942	2.0000	1.4992	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1418.D	QC	ICV	x	16099	2.0000	1.7738	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1413.D	Calibration	5	x	12902	2.0000	1.5018	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1412.D	Calibration	6	x	32065	5.0000	1.4765	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1411.D	Calibration	7	x	65386	10.0000	1.4917	

Calibration Report

Batch Path	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\QuantResults\011422 bna SIM 2.batch.bin	Analyst Name	BL2000\jheine
Analysis Time	2/4/2022 3:29 PM	Reporter Name	BL2000\jheine
Report Time	2/4/2022 3:30:41 PM	Batch State	Processed
Last Calib Update	1/17/2022 8:49 AM	Quant Report Version	10.0
Quant Batch Version	10.0		

Fluorene %RSE = 7.2




Calibration STD Path	Cal Type	Level	Enabled	Resp.	Exp. Conc	Resp. Factor	Level RSD
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1417.D	Calibration	1	x	850	0.1000	2.1334	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1416.D	Calibration	2	x	1584	0.2000	1.9014	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1415.D	Calibration	3	x	3815	0.5000	1.8546	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1414.D	Calibration	4	x	7913	1.0000	1.7778	
\\MASSHUNTER\Org\Data\SV5975.I\sh010421\1 e8270c bna SIM\Jan0402.D	CC	CCV	x	35790	2.0000	1.7340	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1418.D	QC	ICV	x	18411	2.0000	2.0286	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1413.D	Calibration	5	x	15350	2.0000	1.7867	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1412.D	Calibration	6	x	37736	5.0000	1.7377	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1411.D	Calibration	7	x	78747	10.0000	1.7964	

Calibration Report

Batch Path	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\QuantResults\011422 bna SIM 2.batch.bin		
Analysis Time	2/4/2022 3:29 PM	Analyst Name	BL2000\jheine
Report Time	2/4/2022 3:30:41 PM	Reporter Name	BL2000\jheine
Last Calib Update	1/17/2022 8:49 AM	Batch State	Processed
Quant Batch Version	10.0	Quant Report Version	10.0

Phenanthrene %RSE = 2.3

Phenanthrene - 7 Levels, 7 Levels Used, 7 Points, 7 Points Used, 1 QCs




Calibration STD Path	Cal Type	Level	Enabled	Resp.	Exp. Conc	Resp. Factor	Level RSD
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1417.D	Calibration	1	x	1388	0.1000	1.7261	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1416.D	Calibration	2	x	2407	0.2000	1.4221	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1415.D	Calibration	3	x	5535	0.5000	1.3147	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1414.D	Calibration	4	x	11285	1.0000	1.2315	
\\MASSHUNTER\Org\Data\SV5975.I\sh010421\1 e8270c bna SIM\Jan0402.D	CC	CCV	x	54393	2.0000	1.2205	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1418.D	QC	ICV	x	26680	2.0000	1.3898	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1413.D	Calibration	5	x	22214	2.0000	1.2657	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1412.D	Calibration	6	x	54828	5.0000	1.2282	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1411.D	Calibration	7	x	114135	10.0000	1.2757	

Calibration Report

Batch Path	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\QuantResults\011422 bna SIM 2.batch.bin		
Analysis Time	2/4/2022 3:29 PM	Analyst Name	BL2000\jheine
Report Time	2/4/2022 3:30:41 PM	Reporter Name	BL2000\jheine
Last Calib Update	1/17/2022 8:49 AM	Batch State	Processed
Quant Batch Version	10.0	Quant Report Version	10.0

Anthracene %RSE = 1.8




Calibration STD Path	Cal Type	Level	Enabled	Resp.	Exp. Conc	Resp. Factor	Level RSD
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1417.D	Calibration	1	x	1099	0.1000	1.3669	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1416.D	Calibration	2	x	2045	0.2000	1.2080	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1415.D	Calibration	3	x	4750	0.5000	1.1283	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1414.D	Calibration	4	x	9804	1.0000	1.0698	
\\MASSHUNTER\Org\Data\SV5975.I\sh010421\1 e8270c bna SIM\Jan0402.D	CC	CCV	x	45714	2.0000	1.0258	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1418.D	QC	ICV	x	22877	2.0000	1.1917	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1413.D	Calibration	5	x	19299	2.0000	1.0996	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1412.D	Calibration	6	x	49026	5.0000	1.0982	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1411.D	Calibration	7	x	105724	10.0000	1.1817	

Calibration Report

Batch Path	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\QuantResults\011422 bna SIM 2.batch.bin		
Analysis Time	2/4/2022 3:29 PM	Analyst Name	BL2000\jheine
Report Time	2/4/2022 3:30:41 PM	Reporter Name	BL2000\jheine
Last Calib Update	1/17/2022 8:49 AM	Batch State	Processed
Quant Batch Version	10.0	Quant Report Version	10.0

o-Terphenyl %RSE =

o-Terphenyl - 7 Levels, 7 Levels Used, 7 Points, 7 Points Used, 1 QCs




Calibration STD Path	Cal Type	Level	Enabled	Resp.	Exp. Conc	Resp. Factor	Level RSD
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1417.D	Calibration	1	x	615	0.1000	0.7647	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1416.D	Calibration	2	x	1139	0.2000	0.6729	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1415.D	Calibration	3	x	2719	0.5000	0.6459	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1414.D	Calibration	4	x	5628	1.0000	0.6141	
\\MASSHUNTER\Org\Data\SV5975.I\sh010421\1 e8270c bna SIM\Jan0402.D	CC	CCV	x	30546	2.0000	0.6854	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1418.D	QC	ICV	x	13079	2.0000	0.6813	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1413.D	Calibration	5	x	11182	2.0000	0.6372	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1412.D	Calibration	6	x	26874	5.0000	0.6020	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1411.D	Calibration	7	x	55500	10.0000	0.6203	

Calibration Report

Batch Path	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\QuantResults\011422 bna SIM 2.batch.bin	Analyst Name	BL2000\jheine
Analysis Time	2/4/2022 3:29 PM	Reporter Name	BL2000\jheine
Report Time	2/4/2022 3:30:41 PM	Batch State	Processed
Last Calib Update	1/17/2022 8:49 AM	Quant Report Version	10.0
Quant Batch Version	10.0		

Fluoranthene %RSE = 6.0




Calibration STD Path	Cal Type	Level	Enabled	Resp.	Exp. Conc	Resp. Factor	Level RSD
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1417.D	Calibration	1	x	1222	0.1000	1.5188	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1416.D	Calibration	2	x	2335	0.2000	1.3793	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1415.D	Calibration	3	x	5538	0.5000	1.3156	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1414.D	Calibration	4	x	11738	1.0000	1.2809	
\\MASSHUNTER\Org\Data\SV5975.I\sh010421\1 e8270c bna SIM\Jan0402.D	CC	CCV	x	57037	2.0000	1.2799	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1418.D	QC	ICV	x	27466	2.0000	1.4308	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1413.D	Calibration	5	x	22779	2.0000	1.2979	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1412.D	Calibration	6	x	59011	5.0000	1.3219	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1411.D	Calibration	7	x	123634	10.0000	1.3819	

Calibration Report

Batch Path	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\QuantResults\011422 bna SIM 2.batch.bin		
Analysis Time	2/4/2022 3:29 PM	Analyst Name	BL2000\jheine
Report Time	2/4/2022 3:30:42 PM	Reporter Name	BL2000\jheine
Last Calib Update	1/17/2022 8:49 AM	Batch State	Processed
Quant Batch Version	10.0	Quant Report Version	10.0

Pyrene %RSE = 4.8

Pyrene - 7 Levels, 7 Levels Used, 7 Points, 7 Points Used, 1 QCs




Calibration STD Path	Cal Type	Level	Enabled	Resp.	Exp. Conc	Resp. Factor	Level RSD
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1417.D	Calibration	1	x	1310	0.1000	2.1902	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1416.D	Calibration	2	x	2532	0.2000	2.0316	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1415.D	Calibration	3	x	6254	0.5000	2.0040	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1414.D	Calibration	4	x	13080	1.0000	1.9615	
\\MASSHUNTER\Org\Data\SV5975.I\sh010421\1 e8270c bna SIM\Jan0402.D	CC	CCV	x	62808	2.0000	1.9194	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1418.D	QC	ICV	x	30117	2.0000	2.1397	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1413.D	Calibration	5	x	26098	2.0000	1.9982	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1412.D	Calibration	6	x	61779	5.0000	1.8687	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1411.D	Calibration	7	x	135457	10.0000	2.0513	

Calibration Report

Batch Path	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\QuantResults\011422 bna SIM 2.batch.bin		
Analysis Time	2/4/2022 3:29 PM	Analyst Name	BL2000\jheine
Report Time	2/4/2022 3:30:42 PM	Reporter Name	BL2000\jheine
Last Calib Update	1/17/2022 8:49 AM	Batch State	Processed
Quant Batch Version	10.0	Quant Report Version	10.0

Terphenyl-d14 %RSE =




Calibration STD Path	Cal Type	Level	Enabled	Resp.	Exp. Conc	Resp. Factor	Level RSD
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1417.D	Calibration	1	x	584	0.1000	0.9771	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1416.D	Calibration	2	x	1025	0.2000	0.8224	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1415.D	Calibration	3	x	2395	0.5000	0.7675	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1414.D	Calibration	4	x	4851	1.0000	0.7274	
\\MASSHUNTER\Org\Data\SV5975.I\sh010421\1 e8270c bna SIM\Jan0402.D	CC	CCV	x	26408	2.0000	0.8070	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1418.D	QC	ICV	x	9999	2.0000	0.7104	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1413.D	Calibration	5	x	9861	2.0000	0.7551	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1412.D	Calibration	6	x	24394	5.0000	0.7379	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1411.D	Calibration	7	x	50591	10.0000	0.7661	

Calibration Report

Batch Path	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\QuantResults\011422 bna SIM 2.batch.bin		
Analysis Time	2/4/2022 3:29 PM	Analyst Name	BL2000\jheine
Report Time	2/4/2022 3:30:42 PM	Reporter Name	BL2000\jheine
Last Calib Update	1/17/2022 8:49 AM	Batch State	Processed
Quant Batch Version	10.0	Quant Report Version	10.0

Benzo(a)Anthracene %RSE = 3.4

Benzo(a)Anthracene - 7 Levels, 7 Levels Used, 7 Points, 7 Points Used, 1 QCs




Calibration STD Path	Cal Type	Level	Enabled	Resp.	Exp. Conc	Resp. Factor	Level RSD
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1417.D	Calibration	1	x	1860	0.1000	3.1109	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1416.D	Calibration	2	x	2551	0.2000	2.0466	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1415.D	Calibration	3	x	4835	0.5000	1.5491	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1414.D	Calibration	4	x	9011	1.0000	1.3513	
\\MASSHUNTER\Org\Data\SV5975.I\sh010421\1 e8270c bna SIM\Jan0402.D	CC	CCV	x	40166	2.0000	1.2275	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1418.D	QC	ICV	x	20817	2.0000	1.4790	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1413.D	Calibration	5	x	17008	2.0000	1.3023	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1412.D	Calibration	6	x	41708	5.0000	1.2616	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1411.D	Calibration	7	x	90588	10.0000	1.3718	

Calibration Report

Batch Path	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\QuantResults\011422 bna SIM 2.batch.bin	Analyst Name	BL2000\jheine
Analysis Time	2/4/2022 3:29 PM	Reporter Name	BL2000\jheine
Report Time	2/4/2022 3:30:42 PM	Batch State	Processed
Last Calib Update	1/17/2022 8:49 AM	Quant Report Version	10.0
Quant Batch Version	10.0		

Chrysene %RSE = 7.5




Calibration STD Path	Cal Type	Level	Enabled	Resp.	Exp. Conc	Resp. Factor	Level RSD
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1417.D	Calibration	1	x	1172	0.1000	1.9594	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1416.D	Calibration	2	x	2587	0.2000	2.0756	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1415.D	Calibration	3	x	5705	0.5000	1.8282	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1414.D	Calibration	4	x	11797	1.0000	1.7690	
\\MASSHUNTER\Org\Data\SV5975.I\sh010421\1 e8270c bna SIM\Jan0402.D	CC	CCV	x	56647	2.0000	1.7311	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1418.D	QC	ICV	x	27947	2.0000	1.9856	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1413.D	Calibration	5	x	22814	2.0000	1.7468	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1412.D	Calibration	6	x	55864	5.0000	1.6898	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1411.D	Calibration	7	x	115319	10.0000	1.7463	

Calibration Report

Batch Path	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\QuantResults\011422 bna SIM 2.batch.bin	Analyst Name	BL2000\jheine
Analysis Time	2/4/2022 3:29 PM	Reporter Name	BL2000\jheine
Report Time	2/4/2022 3:30:42 PM	Batch State	Processed
Last Calib Update	1/17/2022 8:49 AM	Quant Report Version	10.0
Quant Batch Version	10.0		

Benzo(b)fluoranthene %RSE = 8.4

Benzo(b)fluoranthene - 7 Levels Used, 7 Points, 7 Points Used, 1 QCs




Calibration STD Path	Cal Type	Level	Enabled	Resp.	Exp. Conc	Resp. Factor	Level RSD
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1417.D	Calibration	1	x	754	0.1000	1.9970	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1416.D	Calibration	2	x	1292	0.2000	1.6446	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1415.D	Calibration	3	x	3340	0.5000	1.6473	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1414.D	Calibration	4	x	7329	1.0000	1.6868	
\\MASSHUNTER\Org\Data\SV5975.I\sh010421\1 e8270c bna SIM\Jan0402.D	CC	CCV	x	34226	2.0000	1.6168	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1418.D	QC	ICV	x	19328	2.0000	2.0613	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1413.D	Calibration	5	x	15738	2.0000	1.8220	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1412.D	Calibration	6	x	39707	5.0000	1.8213	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1411.D	Calibration	7	x	88874	10.0000	1.9960	

Calibration Report

Batch Path	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\QuantResults\011422 bna SIM 2.batch.bin	Analyst Name	BL2000\jheine
Analysis Time	2/4/2022 3:29 PM	Reporter Name	BL2000\jheine
Report Time	2/4/2022 3:30:42 PM	Batch State	Processed
Last Calib Update	1/17/2022 8:49 AM	Quant Report Version	10.0
Quant Batch Version	10.0		

Benzo(k)fluoranthene %RSE = 9.8




Calibration STD Path	Cal Type	Level	Enabled	Resp.	Exp. Conc	Resp. Factor	Level RSD
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1417.D	Calibration	1	x	773	0.1000	2.0460	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1416.D	Calibration	2	x	1925	0.2000	2.4507	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1415.D	Calibration	3	x	4090	0.5000	2.0167	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1414.D	Calibration	4	x	8490	1.0000	1.9540	
\\MASSHUNTER\Org\Data\SV5975.I\sh010421\1 e8270c bna SIM\Jan0402.D	CC	CCV	x	39503	2.0000	1.8661	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1418.D	QC	ICV	x	20600	2.0000	2.1971	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1413.D	Calibration	5	x	17813	2.0000	2.0622	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1412.D	Calibration	6	x	46472	5.0000	2.1316	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1411.D	Calibration	7	x	97846	10.0000	2.1975	

Calibration Report

Batch Path	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\QuantResults\011422 bna SIM 2.batch.bin	Analyst Name	BL2000\jheine
Analysis Time	2/4/2022 3:29 PM	Reporter Name	BL2000\jheine
Report Time	2/4/2022 3:30:42 PM	Batch State	Processed
Last Calib Update	1/17/2022 8:49 AM	Quant Report Version	10.0
Quant Batch Version	10.0		

Benzo(a)pyrene %RSE = 2.2

Benzo(a)pyrene - 7 Levels, 7 Levels Used, 7 Points, 7 Points Used, 1 QCs




Calibration STD Path	Cal Type	Level	Enabled	Resp.	Exp. Conc	Resp. Factor	Level RSD
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1417.D	Calibration	1	x	571	0.1000	1.5123	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1416.D	Calibration	2	x	1118	0.2000	1.4235	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1415.D	Calibration	3	x	2788	0.5000	1.3747	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1414.D	Calibration	4	x	5985	1.0000	1.3775	
\\MASSHUNTER\Org\Data\SV5975.I\sh010421\1 e8270c bna SIM\Jan0402.D	CC	CCV	x	27265	2.0000	1.2880	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1418.D	QC	ICV	x	13846	2.0000	1.4767	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1413.D	Calibration	5	x	11949	2.0000	1.3833	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1412.D	Calibration	6	x	31631	5.0000	1.4509	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1411.D	Calibration	7	x	73579	10.0000	1.6525	

Calibration Report

Batch Path	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\QuantResults\011422 bna SIM 2.batch.bin		
Analysis Time	2/4/2022 3:29 PM	Analyst Name	BL2000\jheine
Report Time	2/4/2022 3:30:42 PM	Reporter Name	BL2000\jheine
Last Calib Update	1/17/2022 8:49 AM	Batch State	Processed
Quant Batch Version	10.0	Quant Report Version	10.0

Indeno(1,2,3-cd)pyrene %RSE = 4.0




Calibration STD Path	Cal Type	Level	Enabled	Resp.	Exp. Conc	Resp. Factor	Level RSD
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1417.D	Calibration	1	x	532	0.1000	1.4090	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1416.D	Calibration	2	x	997	0.2000	1.2689	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1415.D	Calibration	3	x	2456	0.5000	1.2110	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1414.D	Calibration	4	x	5490	1.0000	1.2636	
\\MASSHUNTER\Org\Data\SV5975.I\sh010421\1 e8270c bna SIM\Jan0402.D	CC	CCV	x	26047	2.0000	1.2305	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1418.D	QC	ICV	x	13543	2.0000	1.4444	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1413.D	Calibration	5	x	11640	2.0000	1.3475	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1412.D	Calibration	6	x	30611	5.0000	1.4041	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1411.D	Calibration	7	x	70907	10.0000	1.5924	

Calibration Report

Batch Path	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\QuantResults\011422 bna SIM 2.batch.bin		
Analysis Time	2/4/2022 3:29 PM	Analyst Name	BL2000\jheine
Report Time	2/4/2022 3:30:42 PM	Reporter Name	BL2000\jheine
Last Calib Update	1/17/2022 8:49 AM	Batch State	Processed
Quant Batch Version	10.0	Quant Report Version	10.0

Dibenzo(a,h)anthracene %RSE = 7.4

Dibenzo(a,h)anthracene - 7 Levels Used, 7 Points, 7 Points Used, 1 QCs




Calibration STD Path	Cal Type	Level	Enabled	Resp.	Exp. Conc	Resp. Factor	Level RSD
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1417.D	Calibration	1	x	652	0.1000	1.7255	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1416.D	Calibration	2	x	1302	0.2000	1.6575	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1415.D	Calibration	3	x	3015	0.5000	1.4868	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1414.D	Calibration	4	x	6525	1.0000	1.5019	
\\MASSHUNTER\Org\Data\SV5975.I\sh010421\1 e8270c bna SIM\Jan0402.D	CC	CCV	x	28600	2.0000	1.3510	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1418.D	QC	ICV	x	15374	2.0000	1.6396	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1413.D	Calibration	5	x	12569	2.0000	1.4551	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1412.D	Calibration	6	x	35101	5.0000	1.6100	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1411.D	Calibration	7	x	77870	10.0000	1.7488	

Calibration Report

Batch Path	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\QuantResults\011422 bna SIM 2.batch.bin		
Analysis Time	2/4/2022 3:29 PM	Analyst Name	BL2000\jheine
Report Time	2/4/2022 3:30:42 PM	Reporter Name	BL2000\jheine
Last Calib Update	1/17/2022 8:49 AM	Batch State	Processed
Quant Batch Version	10.0	Quant Report Version	10.0

Benzo(g,h,i)perylene %RSE = 5.0

Benzo(g,h,i)perylene - 7 Levels, 7 Levels Used, 7 Points, 7 Points Used, 1 QCs



Calibration STD Path	Cal Type	Level	Enabled	Resp.	Exp. Conc	Resp. Factor	Level RSD
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1417.D	Calibration	1	x	807	0.1000	2.1353	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1416.D	Calibration	2	x	1687	0.2000	2.1468	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1415.D	Calibration	3	x	3877	0.5000	1.9120	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1414.D	Calibration	4	x	8433	1.0000	1.9411	
\\MASSHUNTER\Org\Data\SV5975.I\sh010421\1 e8270c bna SIM\Jan0402.D	CC	CCV	x	40497	2.0000	1.9131	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1418.D	QC	ICV	x	20882	2.0000	2.2271	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1413.D	Calibration	5	x	16676	2.0000	1.9305	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1412.D	Calibration	6	x	42846	5.0000	1.9653	
\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1411.D	Calibration	7	x	97437	10.0000	2.1883	

Initial Calibration Report - GCMS

Method Path
 Method File
 Batch Name \\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\QuantResults\011422 bna SIM 2.batch.bin
 Last Calib Update 1/17/2022 8:49:06 AM

Level Name	Calibration Files	Acq. Date-Time	Level Last Update Time
7	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1411.D	1/14/2022 4:42:22 PM	1/17/2022 8:49:06 AM
6	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1412.D	1/14/2022 5:14:49 PM	1/17/2022 8:49:06 AM
5	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1413.D	1/14/2022 5:47:16 PM	1/17/2022 8:49:06 AM
4	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1414.D	1/14/2022 6:19:44 PM	1/17/2022 8:49:06 AM
3	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1415.D	1/14/2022 6:52:13 PM	1/17/2022 8:49:06 AM
2	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1416.D	1/14/2022 7:24:38 PM	1/17/2022 8:49:06 AM
1	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1417.D	1/14/2022 7:57:03 PM	1/17/2022 8:49:06 AM

Compound	Curve Fit	7	6	5	4	3	2	1	Avg RF	%RSD
I 1,4-Dichlorobenzene-d4										
S Nitrobenzene-d5	Quadratic	1.0843	0.8862	0.7724	0.7196	0.6832	0.6299	0.6985	0.7820	19.953
I Naphthalene-d8										
T Naphthalene	Avg RF	1.3980	1.3298	1.3146	1.3477	1.3850	1.3815	1.5305	1.3839	5.172
T 2-Methylnaphthalene	Avg RF	0.7514	0.7198	0.7672	0.7535	0.7791	0.7863	0.8496	0.7724	5.231
T 1-Methylnaphthalene	Avg RF	0.7740	0.7464	0.7541	0.7701	0.8321	0.8626	0.9631	0.8146	9.586
I Acenaphthene-d10										
S 2-Fluorobiphenyl	Avg RF	1.9466	1.8507	1.8419	1.8115	1.8388	2.0080	2.1613	1.9227	6.575
T Acenaphthylene	Avg RF	2.6211	2.4177	2.3285	2.2344	2.3925	2.4678	2.6975	2.4514	6.586
T Acenaphthene	Avg RF	1.4917	1.4765	1.5018	1.4992	1.4973	1.6355	1.8746	1.5681	9.274
T Fluorene	Avg RF	1.7964	1.7377	1.7867	1.7778	1.8546	1.9014	2.1334	1.8554	7.213
I Phenanthrene-d10										
T Phenanthrene	Quadratic	1.2757	1.2282	1.2657	1.2315	1.3147	1.4221	1.7261	1.3520	13.139
T Anthracene	Quadratic	1.1817	1.0982	1.0996	1.0698	1.1283	1.2080	1.3669	1.1646	8.729
S o-Terphenyl	Avg RF	0.6203	0.6020	0.6372	0.6141	0.6459	0.6729	0.7647	0.6510	8.492
T Fluoranthene	Avg RF	1.3819	1.3219	1.2979	1.2809	1.3156	1.3793	1.5188	1.3566	5.984
I Chrysene-d12										
T Pyrene	Avg RF	2.0513	1.8687	1.9982	1.9615	2.0040	2.0316	2.1902	2.0151	4.835
S Terphenyl-d14	Quadratic	0.7661	0.7379	0.7551	0.7274	0.7675	0.8224	0.9771	0.7933	10.905
T Benzo(a)Anthracene	Quadratic	1.3718	1.2616	1.3023	1.3513	1.5491	2.0466	3.1109	1.7134	39.239
T Chrysene	Avg RF	1.7463	1.6898	1.7468	1.7690	1.8282	2.0756	1.9594	1.8307	7.541
I Perylene-d12										
T Benzo(b)fluoranthene	Avg RF	1.9960	1.8213	1.8220	1.6868	1.6473	1.6446	1.9970	1.8021	8.428
T Benzo(k)fluoranthene	Quadratic	2.1975	2.1316	2.0622	1.9540	2.0167	2.4507	2.0460	2.1227	7.752
T Benzo(a)pyrene	Quadratic	1.6525	1.4509	1.3833	1.3775	1.3747	1.4235	1.5123	1.4535	6.929
T Indeno(1,2,3-cd)pyrene	Quadratic	1.5924	1.4041	1.3475	1.2636	1.2110	1.2689	1.4090	1.3567	9.431
T Dibenzo(a,h)anthracene	Avg RF	1.7488	1.6100	1.4551	1.5019	1.4868	1.6575	1.7255	1.5980	7.436

Initial Calibration Report - GCMS

Compound	Curve Fit	7	6	5	4	3	2	1	Avg RF	%RSD
T Benzo(g,h,i)perylene	Quadratic	2.1883	1.9653	1.9305	1.9411	1.9120	2.1468	2.1353	2.0313	5.883

(RedFont and #) = Outlier Flag; (I) = Internal Standard; (T) = Target; (S) = Surrogate; (M) = Matrix Spike

Compounds with Curve fitting not using Avg Response Factor:

Compound	Curve Fit	Curve Fit Formula	Curve Fit R2
S Nitrobenzene-d5	Quadratic	$y = 1.589092 * x^2 + 0.687886 * x - 1.168947E-004$	0.999945
T Phenanthrene	Quadratic	$y = 0.297227 * x^2 + 1.194008 * x + 0.001285$	0.999856
T Anthracene	Quadratic	$y = 0.576911 * x^2 + 1.031628 * x + 8.776189E-004$	0.999900
S Terphenyl-d14	Quadratic	$y = 0.193096 * x^2 + 0.714548 * x + 6.127830E-004$	0.999868
T Benzo(a)Anthracene	Quadratic	$y = 0.862431 * x^2 + 1.133333 * x + 0.004860$	0.999836
T Benzo(k)fluoranthene	Quadratic	$y = 0.772724 * x^2 + 2.006952 * x + 5.940813E-004$	0.999495
T Benzo(a)pyrene	Quadratic	$y = 1.439543 * x^2 + 1.285741 * x + 6.620839E-004$	0.999907
T Indeno(1,2,3-cd)pyrene	Quadratic	$y = 1.434991 * x^2 + 1.231625 * x + 2.670517E-004$	0.999838
T Benzo(g,h,i)perylene	Quadratic	$y = 1.475535 * x^2 + 1.807345 * x + 0.001163$	0.999791

(RedFont and #) = Outlier Flag; (I) = Internal Standard; (T) = Target; (S) = Surrogate; (M) = Matrix Spike

Quantitative Analysis Results Summary Report

Batch Path	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\QuantResults\011422 bna SIM 2.batch.bin	Analyst Name	BL2000\jheine
Analysis Time	2/4/2022 3:29 PM	Reporter Name	BL2000\jheine
Report Time	2/4/2022 3:46:10 PM	Batch State	Processed
Last Calib Update	1/17/2022 8:49 AM	Quant Report Version	10.0
Quant Batch Version	10.0		

Sequence Table

Data File	sample Name	Sample Type	Vial Position	Inj Vol	Level	Acq Method File
Jan1411.D	14-Jan-22_CAL_7	Cal	2	0.1	7	5975BNASIM
Jan1412.D	14-Jan-22_CAL_6	Cal	3	0.1	6	5975BNASIM
Jan1413.D	14-Jan-22_CAL_5	Cal	4	0.1	5	5975BNASIM
Jan1414.D	14-Jan-22_CAL_4	Cal	5	0.1	4	5975BNASIM
Jan1415.D	14-Jan-22_CAL_3	Cal	6	0.1	3	5975BNASIM
Jan1416.D	14-Jan-22_CAL_2	Cal	7	0.1	2	5975BNASIM
Jan1417.D	14-Jan-22_CAL_1	Cal	8	0.1	1	5975BNASIM
Jan1418.D	14-Jan-22_CCV_18	QC	9	0.1	ICV	5975BNASIM

Quantitation Results

Compound: Nitrobenzene-d5

Data File	Sample Type	ISTD	RT	Resp	ISTD Resp	Resp Ratio	Final Conc	Exp. Conc	Accuracy
Jan1411.D	Calibration	1,4-Dichlorobenzene-d4	5.131	49501	182604	0.2711	9.9976	10.0000	100.0
Jan1412.D	Calibration	1,4-Dichlorobenzene-d4	5.131	20380	183982	0.1108	5.0027	5.0000	100.1
Jan1413.D	Calibration	1,4-Dichlorobenzene-d4	5.143	6699	173466	0.0386	2.0174	2.0000	100.9
Jan1414.D	Calibration	1,4-Dichlorobenzene-d4	5.143	3242	180220	0.0180	0.9957	1.0000	99.6
Jan1415.D	Calibration	1,4-Dichlorobenzene-d4	5.143	1431	167513	0.0085	0.4896	0.5000	97.9
Jan1416.D	Calibration	1,4-Dichlorobenzene-d4	5.156	517	164224	0.0031	0.1879	0.2000	94.0
Jan1417.D	Calibration	1,4-Dichlorobenzene-d4	5.156	285	163131	0.0017	0.1077	0.1000	107.7
Jan1418.D	QC	1,4-Dichlorobenzene-d4	5.143	7442	188496	0.0395	2.0580	2.0000	102.9

Compound: Naphthalene

Data File	Sample Type	ISTD	RT	Resp	ISTD Resp	Resp Ratio	Final Conc	Exp. Conc	Accuracy
Jan1411.D	Calibration	Naphthalene-d8	5.953	113952	326053	0.3495	10.1018	10.0000	101.0
Jan1412.D	Calibration	Naphthalene-d8	5.953	54816	329771	0.1662	4.8046	5.0000	96.1
Jan1413.D	Calibration	Naphthalene-d8	5.953	21057	320346	0.0657	1.8999	2.0000	95.0
Jan1414.D	Calibration	Naphthalene-d8	5.953	11085	329021	0.0337	0.9738	1.0000	97.4
Jan1415.D	Calibration	Naphthalene-d8	5.953	5189	299756	0.0173	0.5004	0.5000	100.1
Jan1416.D	Calibration	Naphthalene-d8	5.953	2073	300080	0.0069	0.1997	0.2000	99.8
Jan1417.D	Calibration	Naphthalene-d8	5.953	1112	290643	0.0038	0.1106	0.1000	110.6
Jan1418.D	QC	Naphthalene-d8	5.953	25149	331274	0.0759	2.1943	2.0000	109.7

Compound: 2-Methylnaphthalene

Data File	Sample Type	ISTD	RT	Resp	ISTD Resp	Resp Ratio	Final Conc	Exp. Conc	Accuracy
Jan1411.D	Calibration	Naphthalene-d8	6.790	61246	326053	0.1878	9.7276	10.0000	97.3
Jan1412.D	Calibration	Naphthalene-d8	6.790	29670	329771	0.0900	4.6594	5.0000	93.2
Jan1413.D	Calibration	Naphthalene-d8	6.790	12288	320346	0.0384	1.9865	2.0000	99.3

Quantitative Analysis Results Summary Report

Compound: 2-Methylnaphthalene

Data File	Sample Type	ISTD	RT	Resp	ISTD Resp	Resp Ratio	Final Conc	Exp. Conc	Accuracy
Jan1414.D	Calibration	Naphthalene-d8	6.790	6198	329021	0.0188	0.9755	1.0000	97.6
Jan1415.D	Calibration	Naphthalene-d8	6.790	2919	299756	0.0097	0.5044	0.5000	100.9
Jan1416.D	Calibration	Naphthalene-d8	6.790	1180	300080	0.0039	0.2036	0.2000	101.8
Jan1417.D	Calibration	Naphthalene-d8	6.790	617	290643	0.0021	0.1100	0.1000	110.0
Jan1418.D	QC	Naphthalene-d8	6.790	15117	331274	0.0456	2.3632	2.0000	118.2

Compound: 1-Methylnaphthalene

Data File	Sample Type	ISTD	RT	Resp	ISTD Resp	Resp Ratio	Final Conc	Exp. Conc	Accuracy
Jan1411.D	Calibration	Naphthalene-d8	6.890	63090	326053	0.1935	9.5010	10.0000	95.0
Jan1412.D	Calibration	Naphthalene-d8	6.890	30767	329771	0.0933	4.5812	5.0000	91.6
Jan1413.D	Calibration	Naphthalene-d8	6.902	12079	320346	0.0377	1.8514	2.0000	92.6
Jan1414.D	Calibration	Naphthalene-d8	6.902	6335	329021	0.0193	0.9454	1.0000	94.5
Jan1415.D	Calibration	Naphthalene-d8	6.902	3118	299756	0.0104	0.5107	0.5000	102.1
Jan1416.D	Calibration	Naphthalene-d8	6.902	1294	300080	0.0043	0.2118	0.2000	105.9
Jan1417.D	Calibration	Naphthalene-d8	6.902	700	290643	0.0024	0.1182	0.1000	118.2
Jan1418.D	QC	Naphthalene-d8	6.890	13812	331274	0.0417	2.0472	2.0000	102.4

Compound: 2-Fluorobiphenyl

Data File	Sample Type	ISTD	RT	Resp	ISTD Resp	Resp Ratio	Final Conc	Exp. Conc	Accuracy
Jan1411.D	Calibration	Acenaphthene-d10	7.252	85326	175338	0.4866	10.1242	10.0000	101.2
Jan1412.D	Calibration	Acenaphthene-d10	7.252	40190	173728	0.2313	4.8128	5.0000	96.3
Jan1413.D	Calibration	Acenaphthene-d10	7.264	15824	171827	0.0921	1.9159	2.0000	95.8
Jan1414.D	Calibration	Acenaphthene-d10	7.264	8063	178036	0.0453	0.9422	1.0000	94.2
Jan1415.D	Calibration	Acenaphthene-d10	7.265	3783	164569	0.0230	0.4782	0.5000	95.6
Jan1416.D	Calibration	Acenaphthene-d10	7.265	1673	166596	0.0100	0.2089	0.2000	104.4
Jan1417.D	Calibration	Acenaphthene-d10	7.264	861	159286	0.0054	0.1124	0.1000	112.4
Jan1418.D	QC	Acenaphthene-d10	7.252	17342	181512	0.0955	1.9877	2.0000	99.4

Compound: Acenaphthylene

Data File	Sample Type	ISTD	RT	Resp	ISTD Resp	Resp Ratio	Final Conc	Exp. Conc	Accuracy
Jan1411.D	Calibration	Acenaphthene-d10	7.826	114894	175338	0.6553	10.6924	10.0000	106.9
Jan1412.D	Calibration	Acenaphthene-d10	7.826	52503	173728	0.3022	4.9314	5.0000	98.6
Jan1413.D	Calibration	Acenaphthene-d10	7.826	20005	171827	0.1164	1.8998	2.0000	95.0
Jan1414.D	Calibration	Acenaphthene-d10	7.826	9945	178036	0.0559	0.9115	1.0000	91.1
Jan1415.D	Calibration	Acenaphthene-d10	7.826	4922	164569	0.0299	0.4880	0.5000	97.6
Jan1416.D	Calibration	Acenaphthene-d10	7.826	2056	166596	0.0123	0.2013	0.2000	100.7
Jan1417.D	Calibration	Acenaphthene-d10	7.826	1074	159286	0.0067	0.1100	0.1000	110.0
Jan1418.D	QC	Acenaphthene-d10	7.826	22902	181512	0.1262	2.0588	2.0000	102.9

Compound: Acenaphthene

Data File	Sample Type	ISTD	RT	Resp	ISTD Resp	Resp Ratio	Final Conc	Exp. Conc	Accuracy
Jan1411.D	Calibration	Acenaphthene-d10	8.038	65386	175338	0.3729	9.5126	10.0000	95.1

Quantitative Analysis Results Summary Report

Compound: Acenaphthene

Data File	Sample Type	ISTD	RT	Resp	ISTD Resp	Resp Ratio	Final Conc	Exp. Conc	Accuracy
Jan1412.D	Calibration	Acenaphthene-d10	8.038	32065	173728	0.1846	4.7081	5.0000	94.2
Jan1413.D	Calibration	Acenaphthene-d10	8.038	12902	171827	0.0751	1.9154	2.0000	95.8
Jan1414.D	Calibration	Acenaphthene-d10	8.038	6673	178036	0.0375	0.9561	1.0000	95.6
Jan1415.D	Calibration	Acenaphthene-d10	8.038	3080	164569	0.0187	0.4774	0.5000	95.5
Jan1416.D	Calibration	Acenaphthene-d10	8.038	1362	166596	0.0082	0.2086	0.2000	104.3
Jan1417.D	Calibration	Acenaphthene-d10	8.038	747	159286	0.0047	0.1195	0.1000	119.5
Jan1418.D	QC	Acenaphthene-d10	8.038	16099	181512	0.0887	2.2624	2.0000	113.1

Compound: Fluorene

Data File	Sample Type	ISTD	RT	Resp	ISTD Resp	Resp Ratio	Final Conc	Exp. Conc	Accuracy
Jan1411.D	Calibration	Acenaphthene-d10	8.661	78747	175338	0.4491	9.6821	10.0000	96.8
Jan1412.D	Calibration	Acenaphthene-d10	8.674	37736	173728	0.2172	4.6828	5.0000	93.7
Jan1413.D	Calibration	Acenaphthene-d10	8.673	15350	171827	0.0893	1.9259	2.0000	96.3
Jan1414.D	Calibration	Acenaphthene-d10	8.673	7913	178036	0.0444	0.9582	1.0000	95.8
Jan1415.D	Calibration	Acenaphthene-d10	8.674	3815	164569	0.0232	0.4998	0.5000	100.0
Jan1416.D	Calibration	Acenaphthene-d10	8.674	1584	166596	0.0095	0.2050	0.2000	102.5
Jan1417.D	Calibration	Acenaphthene-d10	8.673	850	159286	0.0053	0.1150	0.1000	115.0
Jan1418.D	QC	Acenaphthene-d10	8.674	18411	181512	0.1014	2.1867	2.0000	109.3

Compound: Phenanthrene

Data File	Sample Type	ISTD	RT	Resp	ISTD Resp	Resp Ratio	Final Conc	Exp. Conc	Accuracy
Jan1411.D	Calibration	Phenanthrene-d10	9.805	114135	357869	0.3189	10.0168	10.0000	100.2
Jan1412.D	Calibration	Phenanthrene-d10	9.805	54828	357137	0.1535	4.9477	5.0000	99.0
Jan1413.D	Calibration	Phenanthrene-d10	9.805	22214	351005	0.0633	2.0509	2.0000	102.5
Jan1414.D	Calibration	Phenanthrene-d10	9.805	11285	366553	0.0308	0.9824	1.0000	98.2
Jan1415.D	Calibration	Phenanthrene-d10	9.805	5535	336790	0.0164	0.5059	0.5000	101.2
Jan1416.D	Calibration	Phenanthrene-d10	9.805	2407	338512	0.0071	0.1949	0.2000	97.5
Jan1417.D	Calibration	Phenanthrene-d10	9.805	1388	321717	0.0043	0.1015	0.1000	101.5
Jan1418.D	QC	Phenanthrene-d10	9.805	26680	383934	0.0695	2.2533	2.0000	112.7

Compound: Anthracene

Data File	Sample Type	ISTD	RT	Resp	ISTD Resp	Resp Ratio	Final Conc	Exp. Conc	Accuracy
Jan1411.D	Calibration	Phenanthrene-d10	9.867	105724	357869	0.2954	10.0177	10.0000	100.2
Jan1412.D	Calibration	Phenanthrene-d10	9.867	49026	357137	0.1373	4.9466	5.0000	98.9
Jan1413.D	Calibration	Phenanthrene-d10	9.867	19299	351005	0.0550	2.0396	2.0000	102.0
Jan1414.D	Calibration	Phenanthrene-d10	9.867	9804	366553	0.0267	0.9893	1.0000	98.9
Jan1415.D	Calibration	Phenanthrene-d10	9.867	4750	336790	0.0141	0.5092	0.5000	101.8
Jan1416.D	Calibration	Phenanthrene-d10	9.867	2045	338512	0.0060	0.1996	0.2000	99.8
Jan1417.D	Calibration	Phenanthrene-d10	9.867	1099	321717	0.0034	0.0983	0.1000	98.3
Jan1418.D	QC	Phenanthrene-d10	9.867	22877	383934	0.0596	2.2082	2.0000	110.4

Quantitative Analysis Results Summary Report

Compound: o-Terphenyl

Data File	Sample Type	ISTD	RT	Resp	ISTD Resp	Resp Ratio	Final Conc	Exp. Conc	Accuracy
Jan1411.D	Calibration	Phenanthrene-d10	10.299	55500	357869	0.1551	9.5287	10.0000	95.3
Jan1412.D	Calibration	Phenanthrene-d10	10.299	26874	357137	0.0752	4.6234	5.0000	92.5
Jan1413.D	Calibration	Phenanthrene-d10	10.299	11182	351005	0.0319	1.9574	2.0000	97.9
Jan1414.D	Calibration	Phenanthrene-d10	10.311	5628	366553	0.0154	0.9433	1.0000	94.3
Jan1415.D	Calibration	Phenanthrene-d10	10.311	2719	336790	0.0081	0.4960	0.5000	99.2
Jan1416.D	Calibration	Phenanthrene-d10	10.311	1139	338512	0.0034	0.2067	0.2000	103.4
Jan1417.D	Calibration	Phenanthrene-d10	10.311	615	321717	0.0019	0.1175	0.1000	117.5
Jan1418.D	QC	Phenanthrene-d10	10.312	13079	383934	0.0341	2.0930	2.0000	104.7

Compound: Fluoranthene

Data File	Sample Type	ISTD	RT	Resp	ISTD Resp	Resp Ratio	Final Conc	Exp. Conc	Accuracy
Jan1411.D	Calibration	Phenanthrene-d10	11.411	123634	357869	0.3455	10.1863	10.0000	101.9
Jan1412.D	Calibration	Phenanthrene-d10	11.411	59011	357137	0.1652	4.8719	5.0000	97.4
Jan1413.D	Calibration	Phenanthrene-d10	11.411	22779	351005	0.0649	1.9135	2.0000	95.7
Jan1414.D	Calibration	Phenanthrene-d10	11.423	11738	366553	0.0320	0.9442	1.0000	94.4
Jan1415.D	Calibration	Phenanthrene-d10	11.423	5538	336790	0.0164	0.4849	0.5000	97.0
Jan1416.D	Calibration	Phenanthrene-d10	11.435	2335	338512	0.0069	0.2033	0.2000	101.7
Jan1417.D	Calibration	Phenanthrene-d10	11.435	1222	321717	0.0038	0.1120	0.1000	112.0
Jan1418.D	QC	Phenanthrene-d10	11.423	27466	383934	0.0715	2.1093	2.0000	105.5

Compound: Pyrene

Data File	Sample Type	ISTD	RT	Resp	ISTD Resp	Resp Ratio	Final Conc	Exp. Conc	Accuracy
Jan1411.D	Calibration	Chrysene-d12	11.794	135457	264142	0.5128	10.1796	10.0000	101.8
Jan1412.D	Calibration	Chrysene-d12	11.794	61779	264474	0.2336	4.6369	5.0000	92.7
Jan1413.D	Calibration	Chrysene-d12	11.794	26098	261208	0.0999	1.9833	2.0000	99.2
Jan1414.D	Calibration	Chrysene-d12	11.794	13080	266746	0.0490	0.9734	1.0000	97.3
Jan1415.D	Calibration	Chrysene-d12	11.794	6254	249663	0.0251	0.4973	0.5000	99.5
Jan1416.D	Calibration	Chrysene-d12	11.806	2532	249293	0.0102	0.2016	0.2000	100.8
Jan1417.D	Calibration	Chrysene-d12	11.806	1310	239183	0.0055	0.1087	0.1000	108.7
Jan1418.D	QC	Chrysene-d12	11.794	30117	281501	0.1070	2.1237	2.0000	106.2

Compound: Terphenyl-d14

Data File	Sample Type	ISTD	RT	Resp	ISTD Resp	Resp Ratio	Final Conc	Exp. Conc	Accuracy
Jan1411.D	Calibration	Chrysene-d12	12.263	50591	264142	0.1915	10.0104	10.0000	100.1
Jan1412.D	Calibration	Chrysene-d12	12.263	24394	264474	0.0922	4.9627	5.0000	99.3
Jan1413.D	Calibration	Chrysene-d12	12.263	9861	261208	0.0378	2.0507	2.0000	102.5
Jan1414.D	Calibration	Chrysene-d12	12.263	4851	266746	0.0182	0.9772	1.0000	97.7
Jan1415.D	Calibration	Chrysene-d12	12.263	2395	249663	0.0096	0.5010	0.5000	100.2
Jan1416.D	Calibration	Chrysene-d12	12.275	1025	249293	0.0041	0.1956	0.2000	97.8
Jan1417.D	Calibration	Chrysene-d12	12.275	584	239183	0.0024	0.1024	0.1000	102.4
Jan1418.D	QC	Chrysene-d12	12.263	9999	281501	0.0355	1.9290	2.0000	96.5

Quantitative Analysis Results Summary Report

Compound: Benzo(a)Anthracene

Data File	Sample Type	ISTD	RT	Resp	ISTD Resp	Resp Ratio	Final Conc	Exp. Conc	Accuracy
Jan1411.D	Calibration	Chrysene-d12	14.702	90588	264142	0.3430	10.0218	10.0000	100.2
Jan1412.D	Calibration	Chrysene-d12	14.702	41708	264474	0.1577	4.9317	5.0000	98.6
Jan1413.D	Calibration	Chrysene-d12	14.701	17008	261208	0.0651	2.0469	2.0000	102.3
Jan1414.D	Calibration	Chrysene-d12	14.701	9011	266746	0.0338	1.0017	1.0000	100.2
Jan1415.D	Calibration	Chrysene-d12	14.702	4835	249663	0.0194	0.5070	0.5000	101.4
Jan1416.D	Calibration	Chrysene-d12	14.714	2551	249293	0.0102	0.1889	0.2000	94.5
Jan1417.D	Calibration	Chrysene-d12	14.714	1860	239183	0.0078	0.1028	0.1000	102.8
Jan1418.D	QC	Chrysene-d12	14.702	20817	281501	0.0739	2.3347	2.0000	116.7

Compound: Chrysene

Data File	Sample Type	ISTD	RT	Resp	ISTD Resp	Resp Ratio	Final Conc	Exp. Conc	Accuracy
Jan1411.D	Calibration	Chrysene-d12	14.789	115319	264142	0.4366	9.5389	10.0000	95.4
Jan1412.D	Calibration	Chrysene-d12	14.789	55864	264474	0.2112	4.6151	5.0000	92.3
Jan1413.D	Calibration	Chrysene-d12	14.789	22814	261208	0.0873	1.9083	2.0000	95.4
Jan1414.D	Calibration	Chrysene-d12	14.789	11797	266746	0.0442	0.9663	1.0000	96.6
Jan1415.D	Calibration	Chrysene-d12	14.789	5705	249663	0.0229	0.4993	0.5000	99.9
Jan1416.D	Calibration	Chrysene-d12	14.789	2587	249293	0.0104	0.2267	0.2000	113.4
Jan1417.D	Calibration	Chrysene-d12	14.789	1172	239183	0.0049	0.1070	0.1000	107.0
Jan1418.D	QC	Chrysene-d12	14.789	27947	281501	0.0993	2.1692	2.0000	108.5

Compound: Benzo(b)fluoranthene

Data File	Sample Type	ISTD	RT	Resp	ISTD Resp	Resp Ratio	Final Conc	Exp. Conc	Accuracy
Jan1411.D	Calibration	Perylene-d12	17.733	88874	178107	0.4990	11.0755	10.0000	110.8
Jan1412.D	Calibration	Perylene-d12	17.733	39707	174410	0.2277	5.0532	5.0000	101.1
Jan1413.D	Calibration	Perylene-d12	17.733	15738	172756	0.0911	2.0220	2.0000	101.1
Jan1414.D	Calibration	Perylene-d12	17.733	7329	173788	0.0422	0.9360	1.0000	93.6
Jan1415.D	Calibration	Perylene-d12	17.733	3340	162226	0.0206	0.4570	0.5000	91.4
Jan1416.D	Calibration	Perylene-d12	17.733	1292	157130	0.0082	0.1825	0.2000	91.3
Jan1417.D	Calibration	Perylene-d12	17.746	754	151093	0.0050	0.1108	0.1000	110.8
Jan1418.D	QC	Perylene-d12	17.733	19328	187526	0.1031	2.2877	2.0000	114.4

Compound: Benzo(k)fluoranthene

Data File	Sample Type	ISTD	RT	Resp	ISTD Resp	Resp Ratio	Final Conc	Exp. Conc	Accuracy
Jan1411.D	Calibration	Perylene-d12	17.795	97846	178107	0.5494	9.9789	10.0000	99.8
Jan1412.D	Calibration	Perylene-d12	17.795	46472	174410	0.2665	5.0530	5.0000	101.1
Jan1413.D	Calibration	Perylene-d12	17.795	17813	172756	0.1031	2.0045	2.0000	100.2
Jan1414.D	Calibration	Perylene-d12	17.795	8490	173788	0.0488	0.9530	1.0000	95.3
Jan1415.D	Calibration	Perylene-d12	17.795	4090	162226	0.0252	0.4883	0.5000	97.7
Jan1416.D	Calibration	Perylene-d12	17.807	1925	157130	0.0123	0.2319	0.2000	115.9
Jan1417.D	Calibration	Perylene-d12	17.807	773	151093	0.0051	0.0900	0.1000	90.0
Jan1418.D	QC	Perylene-d12	17.795	20600	187526	0.1099	2.1338	2.0000	106.7

Quantitative Analysis Results Summary Report

Compound: Benzo(a)pyrene

Data File	Sample Type	ISTD	RT	Resp	ISTD Resp	Resp Ratio	Final Conc	Exp. Conc	Accuracy
Jan1411.D	Calibration	Perylene-d12	18.376	73579	178107	0.4131	10.0209	10.0000	100.2
Jan1412.D	Calibration	Perylene-d12	18.376	31631	174410	0.1814	4.9389	5.0000	98.8
Jan1413.D	Calibration	Perylene-d12	18.376	11949	172756	0.0692	2.0173	2.0000	100.9
Jan1414.D	Calibration	Perylene-d12	18.376	5985	173788	0.0344	1.0216	1.0000	102.2
Jan1415.D	Calibration	Perylene-d12	18.376	2788	162226	0.0172	0.5068	0.5000	101.4
Jan1416.D	Calibration	Perylene-d12	18.388	1118	157130	0.0071	0.1997	0.2000	99.9
Jan1417.D	Calibration	Perylene-d12	18.388	571	151093	0.0038	0.0968	0.1000	96.8
Jan1418.D	QC	Perylene-d12	18.376	13846	187526	0.0738	2.1474	2.0000	107.4

Compound: Indeno(1,2,3-cd)pyrene

Data File	Sample Type	ISTD	RT	Resp	ISTD Resp	Resp Ratio	Final Conc	Exp. Conc	Accuracy
Jan1411.D	Calibration	Perylene-d12	20.229	70907	178107	0.3981	10.0052	10.0000	100.1
Jan1412.D	Calibration	Perylene-d12	20.229	30611	174410	0.1755	4.9716	5.0000	99.4
Jan1413.D	Calibration	Perylene-d12	20.229	11640	172756	0.0674	2.0564	2.0000	102.8
Jan1414.D	Calibration	Perylene-d12	20.229	5490	173788	0.0316	0.9888	1.0000	98.9
Jan1415.D	Calibration	Perylene-d12	20.229	2456	162226	0.0151	0.4764	0.5000	95.3
Jan1416.D	Calibration	Perylene-d12	20.242	997	157130	0.0063	0.1963	0.2000	98.1
Jan1417.D	Calibration	Perylene-d12	20.241	532	151093	0.0035	0.1054	0.1000	105.4
Jan1418.D	QC	Perylene-d12	20.229	13543	187526	0.0722	2.1963	2.0000	109.8

Compound: Dibenzo(a,h)anthracene

Data File	Sample Type	ISTD	RT	Resp	ISTD Resp	Resp Ratio	Final Conc	Exp. Conc	Accuracy
Jan1411.D	Calibration	Perylene-d12	20.291	77870	178107	0.4372	10.9442	10.0000	109.4
Jan1412.D	Calibration	Perylene-d12	20.291	35101	174410	0.2013	5.0378	5.0000	100.8
Jan1413.D	Calibration	Perylene-d12	20.303	12569	172756	0.0728	1.8212	2.0000	91.1
Jan1414.D	Calibration	Perylene-d12	20.303	6525	173788	0.0375	0.9399	1.0000	94.0
Jan1415.D	Calibration	Perylene-d12	20.303	3015	162226	0.0186	0.4652	0.5000	93.0
Jan1416.D	Calibration	Perylene-d12	20.316	1302	157130	0.0083	0.2075	0.2000	103.7
Jan1417.D	Calibration	Perylene-d12	20.316	652	151093	0.0043	0.1080	0.1000	108.0
Jan1418.D	QC	Perylene-d12	20.303	15374	187526	0.0820	2.0521	2.0000	102.6


Compound: Benzo(g,h,i)perylene

Data File	Sample Type	ISTD	RT	Resp	ISTD Resp	Resp Ratio	Final Conc	Exp. Conc	Accuracy
Jan1411.D	Calibration	Perylene-d12	20.550	97437	178107	0.5471	10.0290	10.0000	100.3
Jan1412.D	Calibration	Perylene-d12	20.563	42846	174410	0.2457	4.9176	5.0000	98.4
Jan1413.D	Calibration	Perylene-d12	20.563	16676	172756	0.0965	2.0267	2.0000	101.3
Jan1414.D	Calibration	Perylene-d12	20.563	8433	173788	0.0485	1.0267	1.0000	102.7
Jan1415.D	Calibration	Perylene-d12	20.563	3877	162226	0.0239	0.4982	0.5000	99.6
Jan1416.D	Calibration	Perylene-d12	20.575	1687	157130	0.0107	0.2109	0.2000	105.5
Jan1417.D	Calibration	Perylene-d12	20.575	807	151093	0.0053	0.0922	0.1000	92.2
Jan1418.D	QC	Perylene-d12	20.563	20882	187526	0.1114	2.3281	2.0000	116.4

Quantitation Results Report (QT Reviewed)

Data File	Jan1411.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/14/2022 4:42:22 PM
Sample Name	14-Jan-22_CAL_7	Instrument	GCMS
Vial	2	Multiplier	1.00
DA Method File		Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011422 bna SIM 2.batch.bin	Last Calib Update	1/17/2022 8:49:06 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.497	152.0	182604	40.0000	ng/ml	0.000
M Naphthalene-d8	5.941	136.0	326053	40.0000	ng/ml	0.000
M Acenaphthene-d10	8.001	164.0	175338	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.780	188.0	357869	40.0000	ng/ml	0.000
M Chrysene-d12	14.727	240.0	264142	40.0000	ng/ml	0.000
M Perylene-d12	18.499	264.0	178107	40.0000	ng/ml	0.000
System Monitoring Compounds						
S Nitrobenzene-d5	5.131	82.0	49501	9.9976	ng/ml	-0.012
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 199.95%	*	
S 2-Fluorobiphenyl	7.252	172.0	85326	10.1242	ng/ml	-0.012
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 202.48%	*	
S o-Terphenyl	10.299	230.0	55500	9.5287	ng/ml	0.000
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = 190.57%	*	
S Terphenyl-d14	12.263	244.0	50591	10.0104	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 200.21%	*	
Target Compounds						
T Naphthalene	5.953	128.0	113952	10.1018	ng/ml	95
T 2-Methylnaphthalene	6.790	141.0	61246	9.7276	ng/ml	93
T 1-Methylnaphthalene	6.890	141.0	63090	9.5010	ng/ml	98
T Acenaphthylene	7.826	152.0	114894	10.6924	ng/ml	97
T Acenaphthene	8.038	154.0	65386	9.5126	ng/ml	99
T Fluorene	8.661	166.0	78747	9.6821	ng/ml	99
T Phenanthrene	9.805	178.0	114135	10.0168	ng/ml	92
T Anthracene	9.867	178.0	105724	10.0177	ng/ml	100
T Fluoranthene	11.411	202.0	123634	10.1863	ng/ml	99
T Pyrene	11.794	202.0	135457	10.1796	ng/ml	98
T Benzo(a)Anthracene	14.702	228.0	90588	10.0218	ng/ml	98
T Chrysene	14.789	228.0	115319	9.5389	ng/ml	99
T Benzo(b)fluoranthene	17.733	252.0	88874	11.0755	ng/ml	99


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	17.795	252.0	97846	9.9789	ng/ml	98
T Benzo(a)pyrene	18.376	252.0	73579	10.0209	ng/ml	100
T Indeno(1,2,3-cd)pyrene	20.229	276.0	70907	10.0052	ng/ml	94
T Dibenzo(a,h)anthracene	20.291	278.0	77870	10.9442	ng/ml	96
T Benzo(g,h,i)perylene	20.550	276.0	97437	10.0290	ng/ml	96


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	9.9976	5.13	-0.01	49501	54.0	35.4	25.9	48.1
					128.0	33.3	25.6	47.6



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	10.1018	5.95	0.00	113952	102.0	16.8	0.0	59.6
					129.0	10.8	7.7	14.3






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	9.7276	6.79	0.00	61246	142.0	149.8	98.5	183.0
					115.0	65.4	41.8	77.6






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	9.5010	6.89	-0.01	63090	142.0	110.1	79.2	147.1
					115.0	68.8	47.5	88.2






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	10.1242	7.25	-0.01	85326	171.0	37.5	26.6	49.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthylene	10.6924	7.83	0.00	114894	153.0	14.1	9.0	16.6






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	9.5126	8.04	0.00	65386	153.0	116.3	82.1	152.6
					152.0	57.4	41.0	76.1






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene	9.6821	8.66	-0.01	78747	165.0 167.0	100.0 13.4	69.1 9.7	128.3 18.0






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Phenanthrene	10.0168	9.81	0.00	114135	176.0	19.0	10.8	20.1



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Anthracene	10.0177	9.87	0.00	105724	176.0	18.3	12.7	23.5




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
o-Terphenyl	9.5287	10.30	0.00	55500	229.0 215.0	70.5 48.0	49.2 32.7	91.3 60.7




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluoranthene	10.1863	11.41	0.00	123634	101.0	13.3	9.6	17.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Pyrene	10.1796	11.79	0.00	135457	101.0	16.1	10.7	20.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	10.0104	12.26	0.00	50591	122.0	20.1	13.4	25.0




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)Anthracene	10.0218	14.70	0.00	90588	226.0	27.5	18.9	35.1
					229.0	21.5	16.1	29.9




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	9.5389	14.79	0.00	115319	226.0 229.0	30.8 20.6	21.2 15.0	39.4 27.8




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(b)fluoranthene	11.0755	17.73	0.00	88874	253.0	22.1	15.8	29.4



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(k)fluoranthene	9.9789	17.80	0.00	97846	253.0	22.2	16.1	29.9



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene	10.0209	18.38	0.00	73579	253.0	23.6	16.5	30.6




Quantitation Results Report (QT Reviewed)

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Indeno(1,2,3-cd)pyrene	10.0052	20.23	0.00	70907	138.0	25.7	20.3	37.6
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1411.D</p> </div> <div style="width: 30%;"> <p>276.0, 138.0</p> <p>Ratio = 25.7 (88.8 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.229-20.229 min, 1 scans) (**) Jan1411.D</p> <p>Lib Match Score=79.3</p> </div> </div>								
Dibenzo(a,h)anthracene	10.9442	20.29	-0.01	77870	279.0	24.7	17.6	32.7
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (278.0) Jan1411.D</p> </div> <div style="width: 30%;"> <p>278.0, 279.0, 139.0</p> <p>Ratio = 24.7 (98.5 %)</p> <p>Ratio = 20.9 (86.5 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.291-20.291 min, 1 scans) (**) Jan1411.D</p> <p>Lib Match Score=77.4</p> </div> </div>								
Benzo(g,h,i)perylene	10.0290	20.55	-0.01	97437	138.0	24.4	19.6	36.5
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1411.D</p> </div> <div style="width: 30%;"> <p>276.0, 138.0, 277.0</p> <p>Ratio = 24.4 (87.2 %)</p> <p>Ratio = 22.7 (97.7 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.550-20.550 min, 1 scans) (**) Jan1411.D</p> <p>Lib Match Score=78.6</p> </div> </div>								

Quantitation Results Report (QT Reviewed)

Data File	Jan1412.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/14/2022 5:14:49 PM
Sample Name	14-Jan-22_CAL_6	Instrument	GCMS
Vial	3	Multiplier	1.00
DA Method File		Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011422 bna SIM 2.batch.bin	Last Calib Update	1/17/2022 8:49:06 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.497	152.0	183982	40.0000	ng/ml	0.000
M Naphthalene-d8	5.928	136.0	329771	40.0000	ng/ml	-0.012
M Acenaphthene-d10	8.001	164.0	173728	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.780	188.0	357137	40.0000	ng/ml	0.000
M Chrysene-d12	14.726	240.0	264474	40.0000	ng/ml	0.000
M Perylene-d12	18.499	264.0	174410	40.0000	ng/ml	0.000
System Monitoring Compounds						
S Nitrobenzene-d5	5.131	82.0	20380	5.0027	ng/ml	-0.012
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 100.05%		
S 2-Fluorobiphenyl	7.252	172.0	40190	4.8128	ng/ml	-0.012
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 96.26%		*
S o-Terphenyl	10.299	230.0	26874	4.6234	ng/ml	0.000
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = 92.47%		
S Terphenyl-d14	12.263	244.0	24394	4.9627	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 99.25%		
Target Compounds						
T Naphthalene	5.953	128.0	54816	4.8046	ng/ml	95
T 2-Methylnaphthalene	6.790	141.0	29670	4.6594	ng/ml	95
T 1-Methylnaphthalene	6.890	141.0	30767	4.5812	ng/ml	99
T Acenaphthylene	7.826	152.0	52503	4.9314	ng/ml	98
T Acenaphthene	8.038	154.0	32065	4.7081	ng/ml	98
T Fluorene	8.674	166.0	37736	4.6828	ng/ml	99
T Phenanthrene	9.805	178.0	54828	4.9477	ng/ml	92
T Anthracene	9.867	178.0	49026	4.9466	ng/ml	100
T Fluoranthene	11.411	202.0	59011	4.8719	ng/ml	98
T Pyrene	11.794	202.0	61779	4.6369	ng/ml	96
T Benzo(a)Anthracene	14.702	228.0	41708	4.9317	ng/ml	99
T Chrysene	14.789	228.0	55864	4.6151	ng/ml	100
T Benzo(b)fluoranthene	17.733	252.0	39707	5.0532	ng/ml	99


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	17.795	252.0	46472	5.0530	ng/ml	99
T Benzo(a)pyrene	18.376	252.0	31631	4.9389	ng/ml	98
T Indeno(1,2,3-cd)pyrene	20.229	276.0	30611	4.9716	ng/ml	99
T Dibenzo(a,h)anthracene	20.291	278.0	35101	5.0378	ng/ml	97
T Benzo(g,h,i)perylene	20.563	276.0	42846	4.9176	ng/ml	98


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	5.0027	5.13	-0.01	20380	54.0	36.3	25.9	48.1
					128.0	27.3	25.6	47.6



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	4.8046	5.95	0.00	54816	102.0	16.5	0.0	59.6
					129.0	10.8	7.7	14.3






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	4.6594	6.79	0.00	29670	142.0	147.4	98.5	183.0
					115.0	63.7	41.8	77.6






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	4.5812	6.89	-0.01	30767	142.0	113.7	79.2	147.1
					115.0	66.6	47.5	88.2






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	4.8128	7.25	-0.01	40190	171.0	37.0	26.6	49.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthylene	4.9314	7.83	0.00	52503	153.0	13.8	9.0	16.6






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	4.7081	8.04	0.00	32065	153.0	115.6	82.1	152.6
					152.0	57.5	41.0	76.1






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene	4.6828	8.67	0.00	37736	165.0	99.5	69.1	128.3
					167.0	13.7	9.7	18.0






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Phenanthrene	4.9477	9.81	0.00	54828	176.0	19.0	10.8	20.1



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Anthracene	4.9466	9.87	0.00	49026	176.0	18.1	12.7	23.5




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
o-Terphenyl	4.6234	10.30	0.00	26874	229.0	70.9	49.2	91.3
					215.0	47.5	32.7	60.7




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluoranthene	4.8719	11.41	0.00	59011	101.0	13.1	9.6	17.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Pyrene	4.6369	11.79	0.00	61779	101.0	16.9	10.7	20.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	4.9627	12.26	0.00	24394	122.0	19.8	13.4	25.0




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)Anthracene	4.9317	14.70	0.00	41708	226.0	27.4	18.9	35.1
					229.0	22.1	16.1	29.9




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	4.6151	14.79	0.00	55864	226.0	30.4	21.2	39.4
					229.0	21.2	15.0	27.8




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(b)fluoranthene	5.0532	17.73	0.00	39707	253.0	22.3	15.8	29.4



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(k)fluoranthene	5.0530	17.80	0.00	46472	253.0	22.3	16.1	29.9



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene	4.9389	18.38	0.00	31631	253.0	24.4	16.5	30.6




Quantitation Results Report (QT Reviewed)

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Indeno(1,2,3-cd)pyrene	4.9716	20.23	0.00	30611	138.0	28.5	20.3	37.6
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1412.D</p> </div> <div style="width: 30%;"> <p>276.0, 138.0</p> <p>Ratio = 28.5 (98.4 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.229-20.229 min, 1 scans) (**) Jan1412.</p> <p>Lib Match Score=78.3</p> </div> </div>								
Dibenzo(a,h)anthracene	5.0378	20.29	-0.01	35101	279.0	24.9	17.6	32.7
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (278.0) Jan1412.D</p> </div> <div style="width: 30%;"> <p>278.0, 279.0, 139.0</p> <p>Ratio = 24.9 (99.0 %)</p> <p>Ratio = 20.9 (86.8 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.291-20.291 min, 1 scans) (**) Jan1412.</p> <p>Lib Match Score=76.3</p> </div> </div>								
Benzo(g,h,i)perylene	4.9176	20.56	0.00	42846	138.0	27.0	19.6	36.5
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1412.D</p> </div> <div style="width: 30%;"> <p>276.0, 138.0, 277.0</p> <p>Ratio = 27.0 (96.1 %)</p> <p>Ratio = 24.3 (104.7 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.563-20.563 min, 1 scans) (**) Jan1412.</p> <p>Lib Match Score=78.3</p> </div> </div>								

Quantitation Results Report (QT Reviewed)

Data File	Jan1413.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/14/2022 5:47:16 PM
Sample Name	14-Jan-22_CAL_5	Instrument	GCMS
Vial	4	Multiplier	1.00
DA Method File		Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011422 bna SIM 2.batch.bin	Last Calib Update	1/17/2022 8:49:06 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.497	152.0	173466	40.0000	ng/ml	0.000
M Naphthalene-d8	5.941	136.0	320346	40.0000	ng/ml	0.000
M Acenaphthene-d10	8.000	164.0	171827	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.780	188.0	351005	40.0000	ng/ml	0.000
M Chrysene-d12	14.726	240.0	261208	40.0000	ng/ml	0.000
M Perylene-d12	18.499	264.0	172756	40.0000	ng/ml	0.000
System Monitoring Compounds						
S Nitrobenzene-d5	5.143	82.0	6699	2.0174	ng/ml	0.000
Spiked Amount: 5.000				Range: 19.0 - 102.0% Recovery = 40.35%		
S 2-Fluorobiphenyl	7.264	172.0	15824	1.9159	ng/ml	0.000
Spiked Amount: 5.000				Range: 25.0 - 94.0% Recovery = 38.32%		
S o-Terphenyl	10.299	230.0	11182	1.9574	ng/ml	0.000
Spiked Amount: 5.000				Range: 40.0 - 140.0% Recovery = 39.15% *		
S Terphenyl-d14	12.263	244.0	9861	2.0507	ng/ml	0.000
Spiked Amount: 5.000				Range: 39.0 - 106.0% Recovery = 41.01%		
Target Compounds						
T Naphthalene	5.953	128.0	21057	1.8999	ng/ml	100
T 2-Methylnaphthalene	6.790	141.0	12288	1.9865	ng/ml	100
T 1-Methylnaphthalene	6.902	141.0	12079	1.8514	ng/ml	100
T Acenaphthylene	7.826	152.0	20005	1.8998	ng/ml	100
T Acenaphthene	8.038	154.0	12902	1.9154	ng/ml	100
T Fluorene	8.673	166.0	15350	1.9259	ng/ml	100
T Phenanthrene	9.805	178.0	22214	2.0509	ng/ml	100
T Anthracene	9.867	178.0	19299	2.0396	ng/ml	100
T Fluoranthene	11.411	202.0	22779	1.9135	ng/ml	100
T Pyrene	11.794	202.0	26098	1.9833	ng/ml	100
T Benzo(a)Anthracene	14.701	228.0	17008	2.0469	ng/ml	100
T Chrysene	14.789	228.0	22814	1.9083	ng/ml	100
T Benzo(b)fluoranthene	17.733	252.0	15738	2.0220	ng/ml	100


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	17.795	252.0	17813	2.0045	ng/ml	100
T Benzo(a)pyrene	18.376	252.0	11949	2.0173	ng/ml	100
T Indeno(1,2,3-cd)pyrene	20.229	276.0	11640	2.0564	ng/ml	100
T Dibenzo(a,h)anthracene	20.303	278.0	12569	1.8212	ng/ml	100
T Benzo(g,h,i)perylene	20.563	276.0	16676	2.0267	ng/ml m	100


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	2.0174	5.14	0.00	6699	54.0	37.0	25.9	48.1
					128.0	36.6	25.6	47.6



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	1.8999	5.95	0.00	21057	102.0	19.9	0.0	59.6
					129.0	11.0	7.7	14.3






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	1.9865	6.79	0.00	12288	142.0	140.8	98.5	183.0
					115.0	59.7	41.8	77.6






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	1.8514	6.90	0.00	12079	142.0	113.1	79.2	147.1
					115.0	67.8	47.5	88.2






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	1.9159	7.26	0.00	15824	171.0	38.0	26.6	49.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthylene	1.8998	7.83	0.00	20005	153.0	12.9	9.0	16.6






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	1.9154	8.04	0.00	12902	153.0	117.4	82.1	152.6
					152.0	58.6	41.0	76.1






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene	1.9259	8.67	0.00	15350	165.0	98.7	69.1	128.3
					167.0	13.9	9.7	18.0






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Phenanthrene	2.0509	9.80	0.00	22214	176.0	15.5	10.8	20.1



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Anthracene	2.0396	9.87	0.00	19299	176.0	18.1	12.7	23.5




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
o-Terphenyl	1.9574	10.30	0.00	11182	229.0	70.2	49.2	91.3
					215.0	46.7	32.7	60.7




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluoranthene	1.9135	11.41	0.00	22779	101.0	13.8	9.6	17.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Pyrene	1.9833	11.79	0.00	26098	101.0	15.3	10.7	20.0















Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	2.0507	12.26	0.00	9861	122.0	19.2	13.4	25.0












Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)Anthracene	2.0469	14.70	0.00	17008	226.0 229.0	27.0 23.0	18.9 16.1	35.1 29.9



Quantitation Results Report (QT Reviewed)

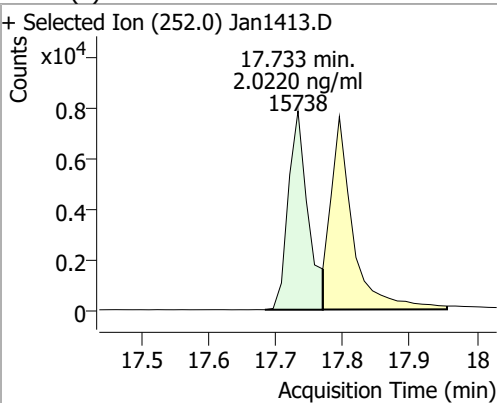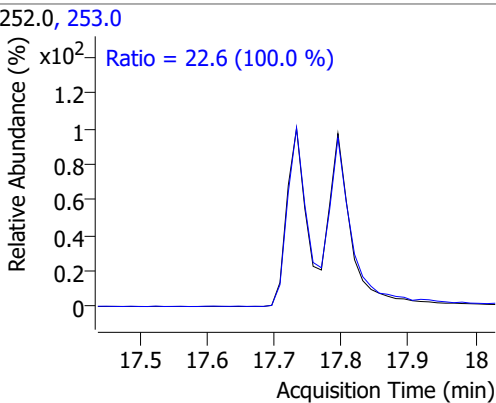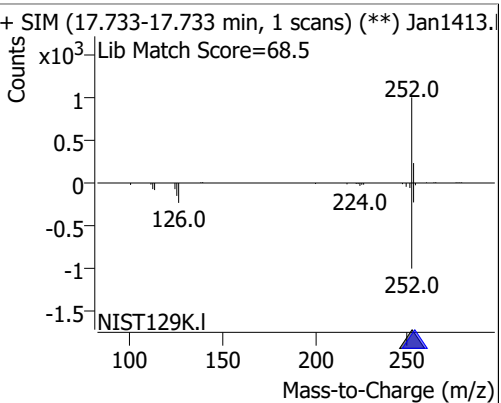Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	1.9083	14.79	0.00	22814	226.0 229.0	30.3 21.4	21.2 15.0	39.4 27.8
+ Selected Ion (228.0) Jan1413.D 			228.0, 226.0, 229.0 			+ SIM (14.789-14.789 min, 1 scans) (**) Jan1413. Lib Match Score=55.4 		
Benzo(b)fluoranthene	2.0220	17.73	0.00	15738	253.0	22.6	15.8	29.4
+ Selected Ion (252.0) Jan1413.D 			252.0, 253.0 			+ SIM (17.733-17.733 min, 1 scans) (**) Jan1413. Lib Match Score=68.5 		
Benzo(k)fluoranthene	2.0045	17.79	0.00	17813	253.0	23.0	16.1	29.9
+ Selected Ion (252.0) Jan1413.D 			252.0, 253.0 			+ SIM (17.795-17.795 min, 1 scans) (**) Jan1413. Lib Match Score=68.5 		
Benzo(a)pyrene	2.0173	18.38	0.00	11949	253.0	23.5	16.5	30.6
+ Selected Ion (252.0) Jan1413.D 			252.0, 253.0 			+ SIM (18.376-18.376 min, 1 scans) (**) Jan1413. Lib Match Score=68.2 		


Quantitation Results Report (QT Reviewed)

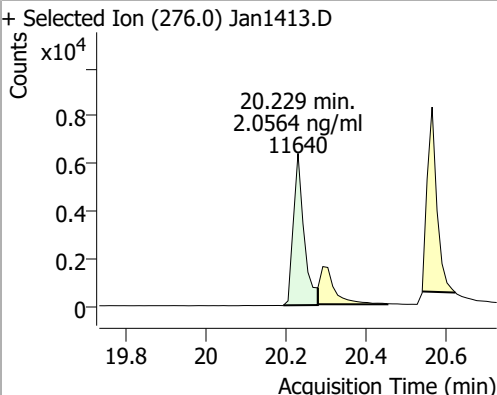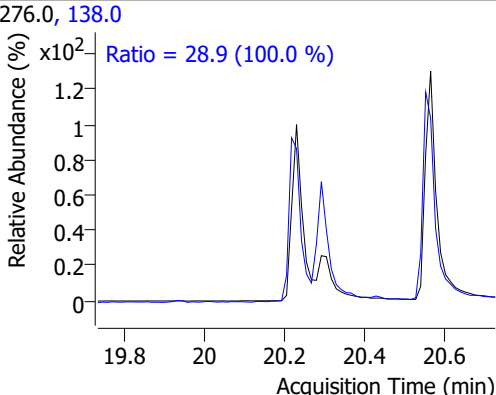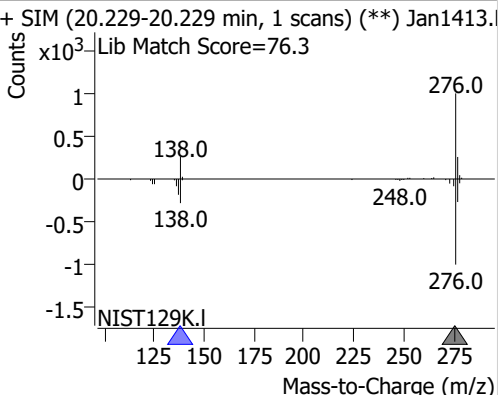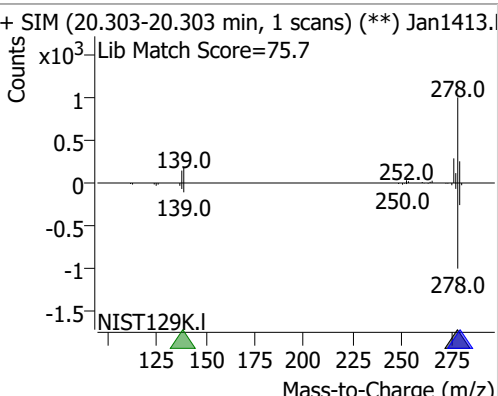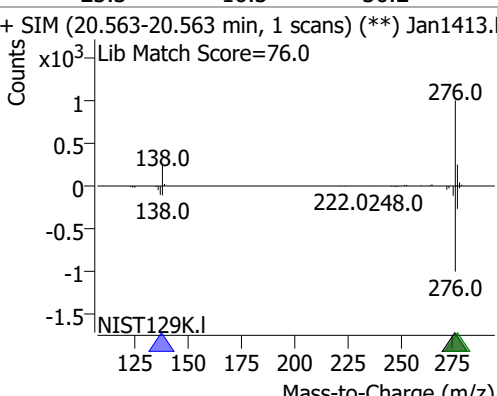Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Indeno(1,2,3-cd)pyrene	2.0564	20.23	0.00	11640	138.0	28.9	20.3	37.6
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1413.D</p>  </div> <div style="width: 30%;"> <p>276.0, 138.0</p> <p>Ratio = 28.9 (100.0 %)</p>  </div> <div style="width: 30%;"> <p>+ SIM (20.229-20.229 min, 1 scans) (**) Jan1413.D</p> <p>Lib Match Score=76.3</p>  </div> </div>								
Dibenzo(a,h)anthracene	1.8212	20.30	0.00	12569	279.0	25.1	17.6	32.7
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (278.0) Jan1413.D</p>  </div> <div style="width: 30%;"> <p>278.0, 279.0, 139.0</p> <p>Ratio = 25.1 (100.0 %)</p> <p>Ratio = 24.1 (100.0 %)</p>  </div> <div style="width: 30%;"> <p>+ SIM (20.303-20.303 min, 1 scans) (**) Jan1413.D</p> <p>Lib Match Score=75.7</p>  </div> </div>								
Benzo(g,h,i)perylene	2.0267	20.56	0.00	16676 (m)	138.0	28.0	19.6	36.5
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1413.D</p>  </div> <div style="width: 30%;"> <p>276.0, 138.0, 277.0</p> <p>Ratio = 28.0 (100.0 %)</p> <p>Ratio = 23.3 (100.0 %)</p>  </div> <div style="width: 30%;"> <p>+ SIM (20.563-20.563 min, 1 scans) (**) Jan1413.D</p> <p>Lib Match Score=76.0</p>  </div> </div>								

Quantitation Results Report (QT Reviewed)

Data File	Jan1414.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/14/2022 6:19:44 PM
Sample Name	14-Jan-22_CAL_4	Instrument	GCMS
Vial	5	Multiplier	1.00
DA Method File		Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011422 bna SIM 2.batch.bin	Last Calib Update	1/17/2022 8:49:06 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.497	152.0	180220	40.0000	ng/ml	0.000
M Naphthalene-d8	5.941	136.0	329021	40.0000	ng/ml	0.000
M Acenaphthene-d10	8.013	164.0	178036	40.0000	ng/ml	0.013
M Phenanthrene-d10	9.780	188.0	366553	40.0000	ng/ml	0.000
M Chrysene-d12	14.726	240.0	266746	40.0000	ng/ml	0.000
M Perylene-d12	18.499	264.0	173788	40.0000	ng/ml	0.000
System Monitoring Compounds						
S Nitrobenzene-d5	5.143	82.0	3242	0.9957	ng/ml	0.000
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 19.91%		
S 2-Fluorobiphenyl	7.264	172.0	8063	0.9422	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 18.84%		*
S o-Terphenyl	10.311	230.0	5628	0.9433	ng/ml	0.012
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = 18.87%		*
S Terphenyl-d14	12.263	244.0	4851	0.9772	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 19.54%		*
Target Compounds						
T Naphthalene	5.953	128.0	11085	0.9738	ng/ml	97
T 2-Methylnaphthalene	6.790	141.0	6198	0.9755	ng/ml	98
T 1-Methylnaphthalene	6.902	141.0	6335	0.9454	ng/ml	99
T Acenaphthylene	7.826	152.0	9945	0.9115	ng/ml	98
T Acenaphthene	8.038	154.0	6673	0.9561	ng/ml	100
T Fluorene	8.673	166.0	7913	0.9582	ng/ml	99
T Phenanthrene	9.805	178.0	11285	0.9824	ng/ml	92
T Anthracene	9.867	178.0	9804	0.9893	ng/ml	99
T Fluoranthene	11.423	202.0	11738	0.9442	ng/ml	99
T Pyrene	11.794	202.0	13080	0.9734	ng/ml	98
T Benzo(a)Anthracene	14.701	228.0	9011	1.0017	ng/ml	98
T Chrysene	14.789	228.0	11797	0.9663	ng/ml	99
T Benzo(b)fluoranthene	17.733	252.0	7329	0.9360	ng/ml	100




Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	17.795	252.0	8490	0.9530	ng/ml	96
T Benzo(a)pyrene	18.376	252.0	5985	1.0216	ng/ml	98
T Indeno(1,2,3-cd)pyrene	20.229	276.0	5490	0.9888	ng/ml	99
T Dibenzo(a,h)anthracene	20.303	278.0	6525	0.9399	ng/ml	99
T Benzo(g,h,i)perylene	20.563	276.0	8433	1.0267	ng/ml	98




(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	0.9957	5.14	0.00	3242	54.0	37.3	25.9	48.1
					128.0	39.3	25.6	47.6



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	0.9738	5.95	0.00	11085	102.0	21.8	0.0	59.6
					129.0	11.2	7.7	14.3




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	0.9755	6.79	0.00	6198	142.0	137.7	98.5	183.0
					115.0	59.7	41.8	77.6




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	0.9454	6.90	0.00	6335	142.0	112.6	79.2	147.1
					115.0	66.6	47.5	88.2




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	0.9422	7.26	0.00	8063	171.0	36.0	26.6	49.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthylene	0.9115	7.83	0.00	9945	153.0	13.5	9.0	16.6






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	0.9561	8.04	0.00	6673	153.0	117.3	82.1	152.6
					152.0	58.1	41.0	76.1






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene	0.9582	8.67	0.00	7913	165.0	99.4	69.1	128.3
					167.0	12.6	9.7	18.0






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Phenanthrene	0.9824	9.80	0.00	11285	176.0	18.8	10.8	20.1
					178.0	18.8	10.8	20.1



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Anthracene	0.9893	9.87	0.00	9804	176.0	18.4	12.7	23.5
					178.0	18.4	12.7	23.5




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
o-Terphenyl	0.9433	10.31	0.01	5628	229.0	70.7	49.2	91.3
					215.0	46.7	32.7	60.7
					230.0	70.7	49.2	91.3




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluoranthene	0.9442	11.42	0.01	11738	101.0	14.1	9.6	17.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Pyrene	0.9734	11.79	0.00	13080	101.0	16.1	10.7	20.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	0.9772	12.26	0.00	4851	122.0	19.8	13.4	25.0




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)Anthracene	1.0017	14.70	0.00	9011	226.0	26.1	18.9	35.1
					229.0	24.4	16.1	29.9




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	0.9663	14.79	0.00	11797	226.0	30.7	21.2	39.4
					229.0	21.7	15.0	27.8




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(b)fluoranthene	0.9360	17.73	0.00	7329	253.0	22.4	15.8	29.4



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(k)fluoranthene	0.9530	17.80	0.00	8490	253.0	21.2	16.1	29.9



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene	1.0216	18.38	0.00	5985	253.0	22.7	16.5	30.6




Quantitation Results Report (QT Reviewed)

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Indeno(1,2,3-cd)pyrene	0.9888	20.23	0.00	5490	138.0	29.7	20.3	37.6
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1414.D</p> </div> <div style="width: 30%;"> <p>276.0, 138.0</p> <p>Ratio = 29.7 (102.6 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.229-20.229 min, 1 scans) (**) Jan1414.D</p> <p>Lib Match Score=73.0</p> </div> </div>								
Dibenzo(a,h)anthracene	0.9399	20.30	0.00	6525	279.0	24.8	17.6	32.7
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (278.0) Jan1414.D</p> </div> <div style="width: 30%;"> <p>278.0, 279.0, 139.0</p> <p>Ratio = 24.8 (98.8 %)</p> <p>Ratio = 23.6 (97.8 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.303-20.303 min, 1 scans) (**) Jan1414.D</p> <p>Lib Match Score=73.8</p> </div> </div>								
Benzo(g,h,i)perylene	1.0267	20.56	0.00	8433	138.0	29.1	19.6	36.5
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1414.D</p> </div> <div style="width: 30%;"> <p>276.0, 138.0, 277.0</p> <p>Ratio = 29.1 (103.7 %)</p> <p>Ratio = 23.9 (102.6 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.563-20.563 min, 1 scans) (**) Jan1414.D</p> <p>Lib Match Score=73.2</p> </div> </div>								

Quantitation Results Report (QT Reviewed)

Data File	Jan1415.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/14/2022 6:52:13 PM
Sample Name	14-Jan-22_CAL_3	Instrument	GCMS
Vial	6	Multiplier	1.00
DA Method File		Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011422 bna SIM 2.batch.bin	Last Calib Update	1/17/2022 8:49:06 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.509	152.0	167513	40.0000	ng/ml	0.013
M Naphthalene-d8	5.941	136.0	299756	40.0000	ng/ml	0.000
M Acenaphthene-d10	8.001	164.0	164569	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.780	188.0	336790	40.0000	ng/ml	0.000
M Chrysene-d12	14.726	240.0	249663	40.0000	ng/ml	0.000
M Perylene-d12	18.499	264.0	162226	40.0000	ng/ml	0.000
System Monitoring Compounds						
S Nitrobenzene-d5	5.143	82.0	1431	0.4896	ng/ml	0.000
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 9.79%	*	
S 2-Fluorobiphenyl	7.265	172.0	3783	0.4782	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 9.56%	*	
S o-Terphenyl	10.311	230.0	2719	0.4960	ng/ml	0.013
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = 9.92%	*	
S Terphenyl-d14	12.263	244.0	2395	0.5010	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 10.02%	*	
Target Compounds						
T Naphthalene	5.953	128.0	5189	0.5004	ng/ml	85
T 2-Methylnaphthalene	6.790	141.0	2919	0.5044	ng/ml	91
T 1-Methylnaphthalene	6.902	141.0	3118	0.5107	ng/ml	m 91
T Acenaphthylene	7.826	152.0	4922	0.4880	ng/ml	98
T Acenaphthene	8.038	154.0	3080	0.4774	ng/ml	99
T Fluorene	8.674	166.0	3815	0.4998	ng/ml	99
T Phenanthrene	9.805	178.0	5535	0.5059	ng/ml	91
T Anthracene	9.867	178.0	4750	0.5092	ng/ml	99
T Fluoranthene	11.423	202.0	5538	0.4849	ng/ml	99
T Pyrene	11.794	202.0	6254	0.4973	ng/ml	99
T Benzo(a)Anthracene	14.702	228.0	4835	0.5070	ng/ml	93
T Chrysene	14.789	228.0	5705	0.4993	ng/ml	99
T Benzo(b)fluoranthene	17.733	252.0	3340	0.4570	ng/ml	99


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	17.795	252.0	4090	0.4883	ng/ml	99
T Benzo(a)pyrene	18.376	252.0	2788	0.5068	ng/ml	93
T Indeno(1,2,3-cd)pyrene	20.229	276.0	2456	0.4764	ng/ml	98
T Dibenzo(a,h)anthracene	20.303	278.0	3015	0.4652	ng/ml	97
T Benzo(g,h,i)perylene	20.563	276.0	3877	0.4982	ng/ml	95


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	0.4896	5.14	0.00	1431	54.0	32.0	25.9	48.1
					128.0	29.2	25.6	47.6



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	0.5004	5.95	0.00	5189	102.0	30.0	0.0	59.6
					129.0	12.0	7.7	14.3






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	0.5044	6.79	0.00	2919	142.0	131.4	98.5	183.0
					115.0	49.7	41.8	77.6






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	0.5107	6.90	0.00	3118 (m)	142.0	109.0	79.2	147.1
					115.0	53.8	47.5	88.2






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	0.4782	7.26	0.00	3783	171.0	37.3	26.6	49.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthylene	0.4880	7.83	0.00	4922	153.0	13.4	9.0	16.6






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	0.4774	8.04	0.00	3080	153.0	117.9	82.1	152.6
					152.0	60.8	41.0	76.1






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene	0.4998	8.67	0.00	3815	165.0 167.0	99.3 13.0	69.1 9.7	128.3 18.0






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Phenanthrene	0.5059	9.81	0.00	5535	176.0	19.4	10.8	20.1



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Anthracene	0.5092	9.87	0.00	4750	176.0	18.4	12.7	23.5




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
o-Terphenyl	0.4960	10.31	0.01	2719	229.0 215.0	68.8 46.5	49.2 32.7	91.3 60.7




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluoranthene	0.4849	11.42	0.01	5538	101.0	14.2	9.6	17.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Pyrene	0.4973	11.79	0.00	6254	101.0	15.7	10.7	20.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	0.5010	12.26	0.00	2395	122.0	20.8	13.4	25.0




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)Anthracene	0.5070	14.70	0.00	4835	226.0	25.1	18.9	35.1
					229.0	27.9	16.1	29.9




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	0.4993	14.79	0.00	5705	226.0 229.0	31.3 21.6	21.2 15.0	39.4 27.8




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(b)fluoranthene	0.4570	17.73	0.00	3340	253.0	22.2	15.8	29.4




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(k)fluoranthene	0.4883	17.80	0.00	4090	253.0	23.7	16.1	29.9



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene	0.5068	18.38	0.00	2788	253.0	20.3	16.5	30.6




Quantitation Results Report (QT Reviewed)



Quantitation Results Report (QT Reviewed)

Data File	Jan1416.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/14/2022 7:24:38 PM
Sample Name	14-Jan-22_CAL_2	Instrument	GCMS
Vial	7	Multiplier	1.00
DA Method File		Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011422 bna SIM 2.batch.bin	Last Calib Update	1/17/2022 8:49:06 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.509	152.0	164224	40.0000	ng/ml	0.013
M Naphthalene-d8	5.941	136.0	300080	40.0000	ng/ml	0.000
M Acenaphthene-d10	8.001	164.0	166596	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.780	188.0	338512	40.0000	ng/ml	0.000
M Chrysene-d12	14.726	240.0	249293	40.0000	ng/ml	0.000
M Perylene-d12	18.499	264.0	157130	40.0000	ng/ml	0.000
System Monitoring Compounds						
S Nitrobenzene-d5	5.156	82.0	517	0.1879	ng/ml	0.013
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 3.76%	*	
S 2-Fluorobiphenyl	7.265	172.0	1673	0.2089	ng/ml	0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 4.18%	*	
S o-Terphenyl	10.311	230.0	1139	0.2067	ng/ml	0.013
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = 4.13%	*	
S Terphenyl-d14	12.275	244.0	1025	0.1956	ng/ml	0.013
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 3.91%	*	
Target Compounds						
T Naphthalene	5.953	128.0	2073	0.1997	ng/ml	# 50
T 2-Methylnaphthalene	6.790	141.0	1180	0.2036	ng/ml	93
T 1-Methylnaphthalene	6.902	141.0	1294	0.2118	ng/ml	90
T Acenaphthylene	7.826	152.0	2056	0.2013	ng/ml	99
T Acenaphthene	8.038	154.0	1362	0.2086	ng/ml	m 99
T Fluorene	8.674	166.0	1584	0.2050	ng/ml	99
T Phenanthrene	9.805	178.0	2407	0.1949	ng/ml	m 93
T Anthracene	9.867	178.0	2045	0.1996	ng/ml	m 99
T Fluoranthene	11.435	202.0	2335	0.2033	ng/ml	100
T Pyrene	11.806	202.0	2532	0.2016	ng/ml	97
T Benzo(a)Anthracene	14.714	228.0	2551	0.1889	ng/ml	# 89
T Chrysene	14.789	228.0	2587	0.2267	ng/ml	96
T Benzo(b)fluoranthene	17.733	252.0	1292	0.1825	ng/ml	97




Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	17.807	252.0	1925	0.2319	ng/ml	96
T Benzo(a)pyrene	18.388	252.0	1118	0.1997	ng/ml	95
T Indeno(1,2,3-cd)pyrene	20.242	276.0	997	0.1963	ng/ml	96
T Dibenzo(a,h)anthracene	20.316	278.0	1302	0.2075	ng/ml	94
T Benzo(g,h,i)perylene	20.575	276.0	1687	0.2109	ng/ml	98




(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	0.1879	5.16	0.01	517	54.0 128.0	34.5 31.0	25.9 25.6	48.1 47.6



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	0.1997	5.95	0.00	2073	102.0 129.0	52.9 14.5	0.0 7.7	59.6 14.3






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	0.2036	6.79	0.00	1180	142.0 115.0	129.9 60.6	98.5 41.8	183.0 77.6






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	0.2118	6.90	0.00	1294	142.0	125.9	79.2	147.1
					115.0	62.0	47.5	88.2






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	0.2089	7.26	0.00	1673	171.0	31.8	26.6	49.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthylene	0.2013	7.83	0.00	2056	153.0	12.5	9.0	16.6






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	0.2086	8.04	0.00	1362 (m)	153.0	118.3	82.1	152.6
					152.0	57.6	41.0	76.1






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene	0.2050	8.67	0.00	1584	165.0	97.9	69.1	128.3
					167.0	13.4	9.7	18.0






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Phenanthrene	0.1949	9.81	0.00	2407 (m)	176.0	18.6	10.8	20.1



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Anthracene	0.1996	9.87	0.00	2045 (m)	176.0	18.7	12.7	23.5




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
o-Terphenyl	0.2067	10.31	0.01	1139	229.0	72.1	49.2	91.3
					215.0	47.8	32.7	60.7




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluoranthene	0.2033	11.44	0.02	2335	101.0	13.7	9.6	17.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Pyrene	0.2016	11.81	0.01	2532	101.0	16.5	10.7	20.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	0.1956	12.28	0.01	1025	122.0	19.4	13.4	25.0




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)Anthracene	0.1889	14.71	0.01	2551	226.0	22.8	18.9	35.1
					229.0	30.3	16.1	29.9




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	0.2267	14.79	0.00	2587	226.0	30.2	21.2	39.4
					229.0	17.0	15.0	27.8




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(b)fluoranthene	0.1825	17.73	0.00	1292	253.0	21.0	15.8	29.4












Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(k)fluoranthene	0.2319	17.81	0.01	1925	253.0	21.2	16.1	29.9



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene	0.1997	18.39	0.01	1118	253.0	20.9	16.5	30.6




Quantitation Results Report (QT Reviewed)

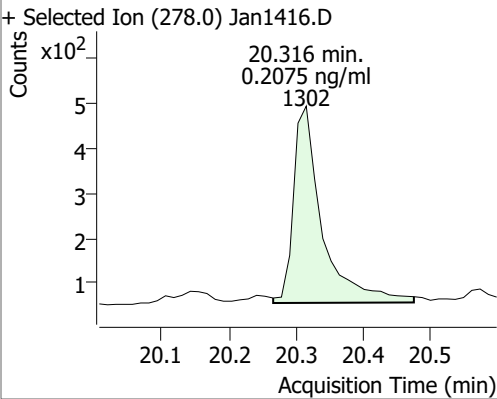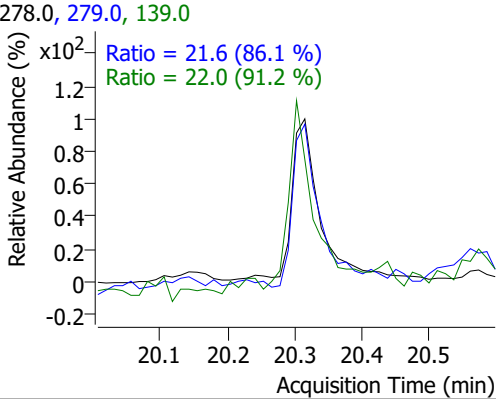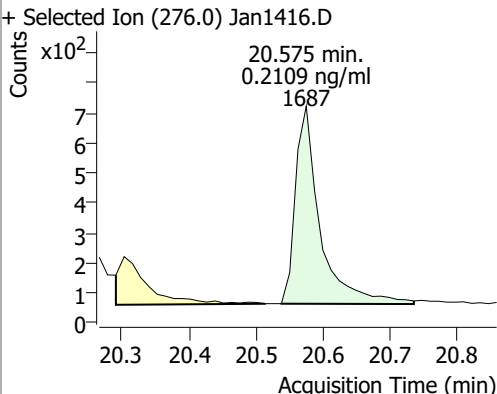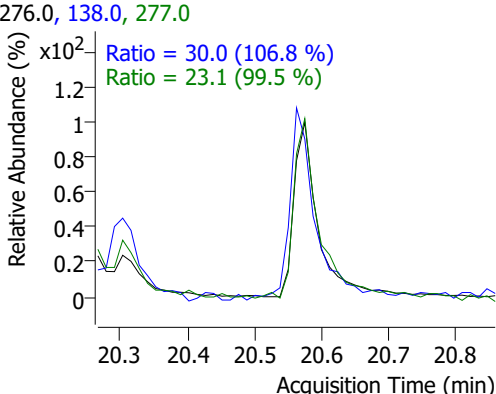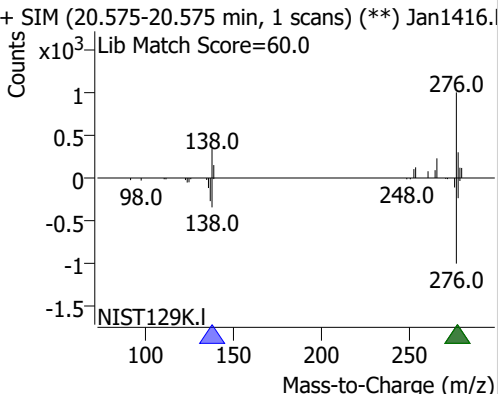Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Indeno(1,2,3-cd)pyrene	0.1963	20.24	0.01	997	138.0	26.9	20.3	37.6
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1416.D</p>  </div> <div style="width: 30%;"> <p>276.0, 138.0</p> <p>Ratio = 26.9 (93.1 %)</p>  </div> <div style="width: 30%;"> <p>+ SIM (20.242-20.242 min, 1 scans) (**) Jan1416.D</p> <p>Lib Match Score=59.4</p>  </div> </div>								
Dibenzo(a,h)anthracene	0.2075	20.32	0.01	1302	279.0	21.6	17.6	32.7
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (278.0) Jan1416.D</p>  </div> <div style="width: 30%;"> <p>278.0, 279.0, 139.0</p> <p>Ratio = 21.6 (86.1 %)</p> <p>Ratio = 22.0 (91.2 %)</p>  </div> <div style="width: 30%;"> <p>+ SIM (20.316-20.316 min, 1 scans) (**) Jan1416.D</p> <p>Lib Match Score=63.5</p>  </div> </div>								
Benzo(g,h,i)perylene	0.2109	20.58	0.01	1687	138.0	30.0	19.6	36.5
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1416.D</p>  </div> <div style="width: 30%;"> <p>276.0, 138.0, 277.0</p> <p>Ratio = 30.0 (106.8 %)</p> <p>Ratio = 23.1 (99.5 %)</p>  </div> <div style="width: 30%;"> <p>+ SIM (20.575-20.575 min, 1 scans) (**) Jan1416.D</p> <p>Lib Match Score=60.0</p>  </div> </div>								

Quantitation Results Report (QT Reviewed)

Data File	Jan1417.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/14/2022 7:57:03 PM
Sample Name	14-Jan-22_CAL_1	Instrument	GCMS
Vial	8	Multiplier	1.00
DA Method File		Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011422 bna SIM 2.batch.bin	Last Calib Update	1/17/2022 8:49:06 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.509	152.0	163131	40.0000	ng/ml	0.012
M Naphthalene-d8	5.941	136.0	290643	40.0000	ng/ml	0.000
M Acenaphthene-d10	8.013	164.0	159286	40.0000	ng/ml	0.013
M Phenanthrene-d10	9.780	188.0	321717	40.0000	ng/ml	0.000
M Chrysene-d12	14.726	240.0	239183	40.0000	ng/ml	0.000
M Perylene-d12	18.499	264.0	151093	40.0000	ng/ml	0.000
System Monitoring Compounds						
S Nitrobenzene-d5	5.156	82.0	285	0.1077	ng/ml	#m 0.012
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 2.15%		*
S 2-Fluorobiphenyl	7.264	172.0	861	0.1124	ng/ml	m 0.000
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 2.25%		*
S o-Terphenyl	10.311	230.0	615	0.1175	ng/ml	m 0.012
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = 2.35%		*
S Terphenyl-d14	12.275	244.0	584	0.1024	ng/ml	m 0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 2.05%		*
Target Compounds						
T Naphthalene	5.953	128.0	1112	0.1106	ng/ml	# 67
T 2-Methylnaphthalene	6.790	141.0	617	0.1100	ng/ml	82
T 1-Methylnaphthalene	6.902	141.0	700	0.1182	ng/ml	94
T Acenaphthylene	7.826	152.0	1074	0.1100	ng/ml	93
T Acenaphthene	8.038	154.0	747	0.1195	ng/ml	m 88
T Fluorene	8.673	166.0	850	0.1150	ng/ml	97
T Phenanthrene	9.805	178.0	1388	0.1015	ng/ml	98
T Anthracene	9.867	178.0	1099	0.0983	ng/ml	99
T Fluoranthene	11.435	202.0	1222	0.1120	ng/ml	m 100
T Pyrene	11.806	202.0	1310	0.1087	ng/ml	m 98
T Benzo(a)Anthracene	14.714	228.0	1860	0.1028	ng/ml	#m 85
T Chrysene	14.789	228.0	1172	0.1070	ng/ml	m 97
T Benzo(b)fluoranthene	17.746	252.0	754	0.1108	ng/ml	97


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	17.807	252.0	773	0.0900	ng/ml	m 92
T Benzo(a)pyrene	18.388	252.0	571	0.0968	ng/ml	m 93
T Indeno(1,2,3-cd)pyrene	20.241	276.0	532	0.1054	ng/ml	95
T Dibenzo(a,h)anthracene	20.316	278.0	652	0.1080	ng/ml	98
T Benzo(g,h,i)perylene	20.575	276.0	807	0.0922	ng/ml	#m 81


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	0.1077	5.16	0.01	285 (m)	54.0 128.0	26.4 21.3	25.9 25.6	48.1 47.6



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	0.1106	5.95	0.00	1112	102.0 129.0	38.9 17.6	0.0 7.7	59.6 14.3






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	0.1100	6.79	0.00	617	142.0 115.0	112.0 54.8	98.5 41.8	183.0 77.6






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	0.1182	6.90	0.00	700	142.0	117.5	79.2	147.1
					115.0	59.4	47.5	88.2






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	0.1124	7.26	0.00	861 (m)	171.0	38.2	26.6	49.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthylene	0.1100	7.83	0.00	1074	153.0	10.2	9.0	16.6






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	0.1195	8.04	0.00	747 (m)	153.0	98.5	82.1	152.6
					152.0	56.6	41.0	76.1






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene	0.1150	8.67	0.00	850	165.0	102.2	69.1	128.3
					167.0	13.3	9.7	18.0






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Phenanthrene	0.1015	9.80	0.00	1388	176.0	16.4	10.8	20.1



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Anthracene	0.0983	9.87	0.00	1099	176.0	17.5	12.7	23.5




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
o-Terphenyl	0.1175	10.31	0.01	615 (m)	229.0	65.3	49.2	91.3
					215.0	44.0	32.7	60.7




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluoranthene	0.1120	11.44	0.02	1222 (m)	101.0	13.9	9.6	17.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Pyrene	0.1087	11.81	0.01	1310 (m)	101.0	14.4	10.7	20.0















Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	0.1024	12.28	0.01	584	122.0	19.2	13.4	25.0












Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)Anthracene	0.1028	14.71	0.01	1860 (m)	226.0 229.0	20.7 32.0	18.9 16.1	35.1 29.9



Quantitation Results Report (QT Reviewed)

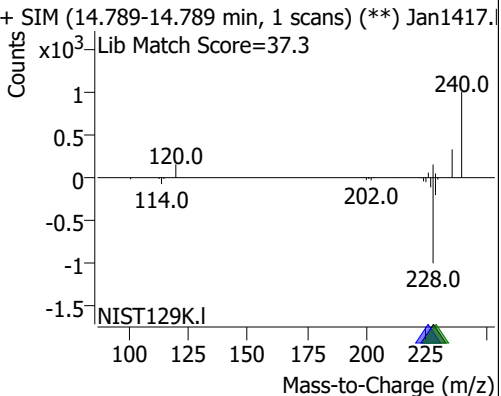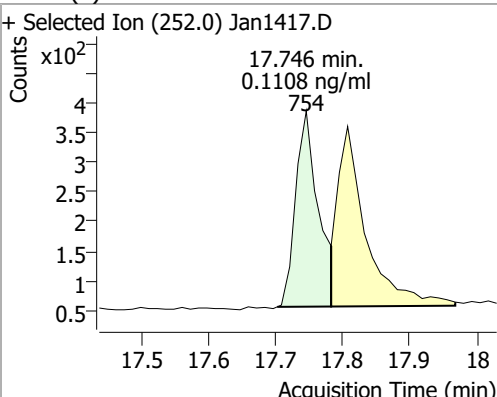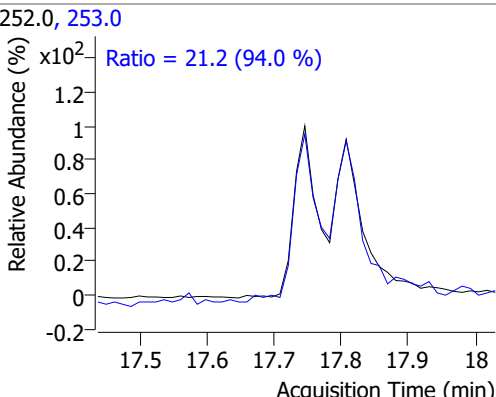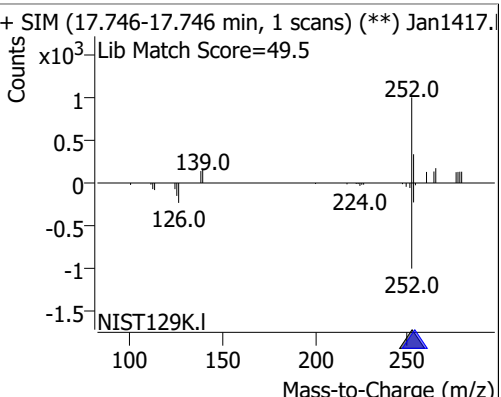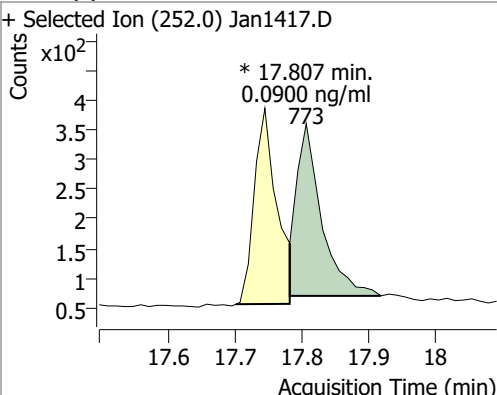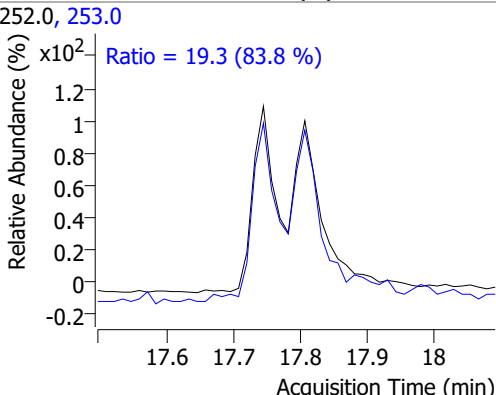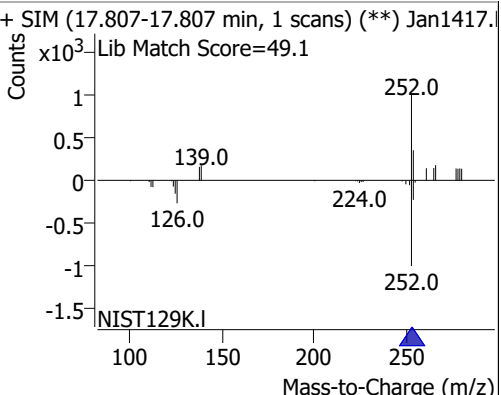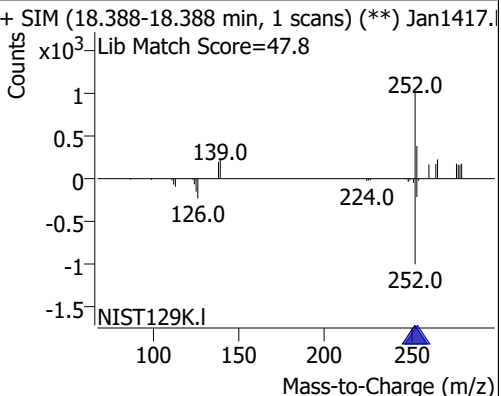Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	0.1070	14.79	0.00	1172 (m)	226.0 229.0	31.8 22.4	21.2 15.0	39.4 27.8
+ Selected Ion (228.0) Jan1417.D			228.0, 226.0, 229.0			+ SIM (14.789-14.789 min, 1 scans) (**) Jan1417.1		
								
Benzo(b)fluoranthene	0.1108	17.75	0.01	754	253.0	21.2	15.8	29.4
+ Selected Ion (252.0) Jan1417.D			252.0, 253.0			+ SIM (17.746-17.746 min, 1 scans) (**) Jan1417.1		
								
Benzo(k)fluoranthene	0.0900	17.81	0.01	773 (m)	253.0	19.3	16.1	29.9
+ Selected Ion (252.0) Jan1417.D			252.0, 253.0			+ SIM (17.807-17.807 min, 1 scans) (**) Jan1417.1		
								
Benzo(a)pyrene	0.0968	18.39	0.01	571 (m)	253.0	20.2	16.5	30.6
+ Selected Ion (252.0) Jan1417.D			252.0, 253.0			+ SIM (18.388-18.388 min, 1 scans) (**) Jan1417.1		
								


Quantitation Results Report (QT Reviewed)

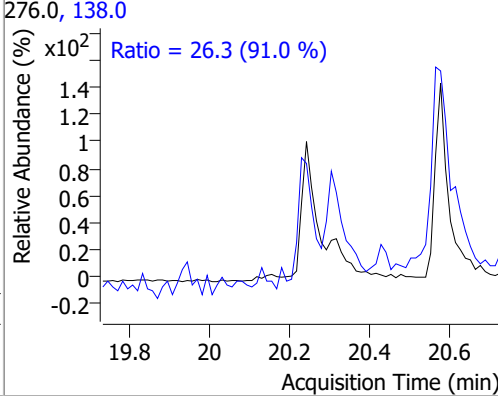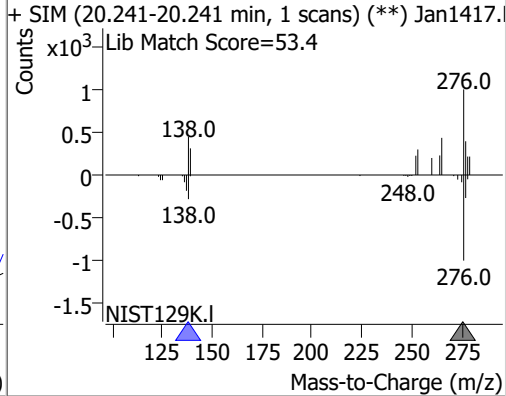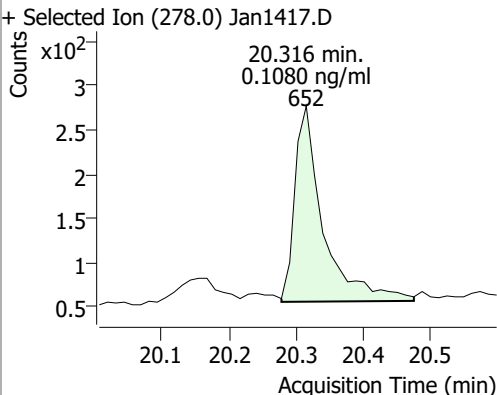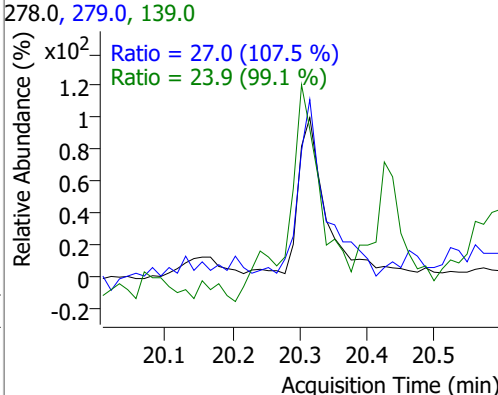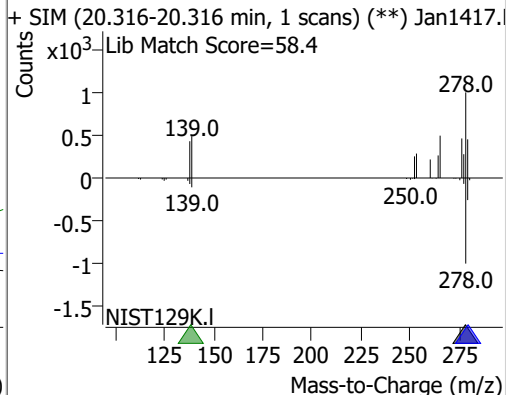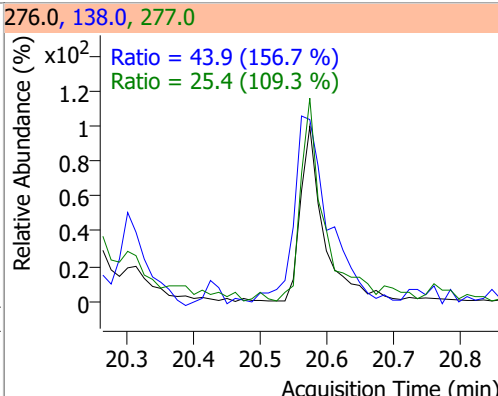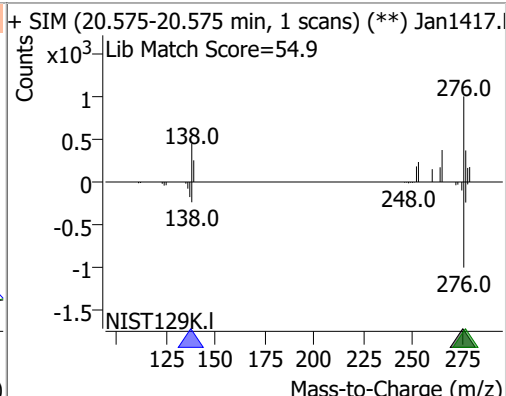Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Indeno(1,2,3-cd)pyrene	0.1054	20.24	0.01	532	138.0	26.3	20.3	37.6
+ Selected Ion (276.0) Jan1417.D			276.0, 138.0			+ SIM (20.241-20.241 min, 1 scans) (**) Jan1417.0		
								
Dibenzo(a,h)anthracene	0.1080	20.32	0.01	652	279.0	27.0	17.6	32.7
+ Selected Ion (278.0) Jan1417.D			278.0, 279.0, 139.0			+ SIM (20.316-20.316 min, 1 scans) (**) Jan1417.0		
								
Benzo(g,h,i)perylene	0.0922	20.58	0.01	807 (m)	138.0	43.9	19.6	36.5
+ Selected Ion (276.0) Jan1417.D			276.0, 138.0, 277.0			+ SIM (20.575-20.575 min, 1 scans) (**) Jan1417.0		
								

Quantitation Results Report (QT Reviewed)

Data File	Jan1418.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/14/2022 8:29:26 PM
Sample Name	14-Jan-22_CCV_18	Instrument	GCMS
Vial	9	Multiplier	1.00
DA Method File		Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011422 bna SIM 2.batch.bin	Last Calib Update	1/17/2022 8:49:06 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.497	152.0	188496	40.0000	ng/ml	0.000
M Naphthalene-d8	5.941	136.0	331274	40.0000	ng/ml	0.000
M Acenaphthene-d10	8.013	164.0	181512	40.0000	ng/ml	0.013
M Phenanthrene-d10	9.780	188.0	383934	40.0000	ng/ml	0.000
M Chrysene-d12	14.727	240.0	281501	40.0000	ng/ml	0.000
M Perylene-d12	18.499	264.0	187526	40.0000	ng/ml	0.000
System Monitoring Compounds						
S Nitrobenzene-d5	5.143	82.0	7442	2.0580	ng/ml	0.000
Spiked Amount: 5.000	Range: 19.0 - 102.0%		Recovery = 41.16%			
S 2-Fluorobiphenyl	7.252	172.0	17342	1.9877	ng/ml	-0.012
Spiked Amount: 5.000	Range: 25.0 - 94.0%		Recovery = 39.75%			
S o-Terphenyl	10.312	230.0	13079	2.0930	ng/ml	0.013
Spiked Amount: 5.000	Range: 40.0 - 140.0%		Recovery = 41.86%			
S Terphenyl-d14	12.263	244.0	9999	1.9290	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%		Recovery = 38.58%		*	
Target Compounds						
T Naphthalene	5.953	128.0	25149	2.1943	ng/ml	99
T 2-Methylnaphthalene	6.790	141.0	15117	2.3632	ng/ml	m 100
T 1-Methylnaphthalene	6.890	141.0	13812	2.0472	ng/ml	m 98
T Acenaphthylene	7.826	152.0	22902	2.0588	ng/ml	99
T Acenaphthene	8.038	154.0	16099	2.2624	ng/ml	99
T Fluorene	8.674	166.0	18411	2.1867	ng/ml	100
T Phenanthrene	9.805	178.0	26680	2.2533	ng/ml	91
T Anthracene	9.867	178.0	22877	2.2082	ng/ml	100
T Fluoranthene	11.423	202.0	27466	2.1093	ng/ml	100
T Pyrene	11.794	202.0	30117	2.1237	ng/ml	99
T Benzo(a)Anthracene	14.702	228.0	20817	2.3347	ng/ml	100
T Chrysene	14.789	228.0	27947	2.1692	ng/ml	99
T Benzo(b)fluoranthene	17.733	252.0	19328	2.2877	ng/ml	98


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	17.795	252.0	20600	2.1338	ng/ml	100
T Benzo(a)pyrene	18.376	252.0	13846	2.1474	ng/ml	99
T Indeno(1,2,3-cd)pyrene	20.229	276.0	13543	2.1963	ng/ml	98
T Dibenzo(a,h)anthracene	20.303	278.0	15374	2.0521	ng/ml	98
T Benzo(g,h,i)perylene	20.563	276.0	20882	2.3281	ng/ml	98


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	2.0580	5.14	0.00	7442	54.0	36.5	25.9	48.1
					128.0	35.2	25.6	47.6



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	2.1943	5.95	0.00	25149	102.0	19.5	0.0	59.6
					129.0	11.2	7.7	14.3






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	2.3632	6.79	0.00	15117 (m)	142.0	140.4	98.5	183.0
					115.0	60.1	41.8	77.6






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	2.0472	6.89	-0.01	13812 (m)	142.0	111.8	79.2	147.1
					115.0	69.4	47.5	88.2






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	1.9877	7.25	-0.01	17342	171.0	37.9	26.6	49.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthylene	2.0588	7.83	0.00	22902	153.0	13.1	9.0	16.6






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	2.2624	8.04	0.00	16099	153.0	118.0	82.1	152.6
					152.0	59.0	41.0	76.1






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene	2.1867	8.67	0.00	18411	165.0	98.2	69.1	128.3
					167.0	13.9	9.7	18.0






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Phenanthrene	2.2533	9.81	0.00	26680	176.0	19.1	10.8	20.1



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Anthracene	2.2082	9.87	0.00	22877	176.0	18.2	12.7	23.5




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
o-Terphenyl	2.0930	10.31	0.01	13079	229.0	72.4	49.2	91.3
					215.0	47.2	32.7	60.7




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluoranthene	2.1093	11.42	0.01	27466	101.0	14.0	9.6	17.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Pyrene	2.1237	11.79	0.00	30117	101.0	15.8	10.7	20.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	1.9290	12.26	0.00	9999	122.0	18.9	13.4	25.0




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)Anthracene	2.3347	14.70	0.00	20817	226.0	27.2	18.9	35.1
					229.0	22.9	16.1	29.9




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	2.1692	14.79	0.00	27947	226.0	31.0	21.2	39.4
					229.0	21.7	15.0	27.8




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(b)fluoranthene	2.2877	17.73	0.00	19328	253.0	21.7	15.8	29.4



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(k)fluoranthene	2.1338	17.80	0.00	20600	253.0	22.9	16.1	29.9



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene	2.1474	18.38	0.00	13846	253.0	24.1	16.5	30.6




Quantitation Results Report (QT Reviewed)

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Indeno(1,2,3-cd)pyrene	2.1963	20.23	0.00	13543	138.0	27.7	20.3	37.6
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1418.D</p> </div> <div style="width: 30%;"> <p>276.0, 138.0</p> <p>Ratio = 27.7 (95.8 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.229-20.229 min, 1 scans) (**) Jan1418.D</p> <p>Lib Match Score=76.7</p> </div> </div>								
Dibenzo(a,h)anthracene	2.0521	20.30	0.00	15374	279.0	24.1	17.6	32.7
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (278.0) Jan1418.D</p> </div> <div style="width: 30%;"> <p>278.0, 279.0, 139.0</p> <p>Ratio = 24.1 (96.1 %)</p> <p>Ratio = 23.0 (95.4 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.303-20.303 min, 1 scans) (**) Jan1418.D</p> <p>Lib Match Score=76.5</p> </div> </div>								
Benzo(g,h,i)perylene	2.3281	20.56	0.00	20882	138.0	26.7	19.6	36.5
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1418.D</p> </div> <div style="width: 30%;"> <p>276.0, 138.0, 277.0</p> <p>Ratio = 26.7 (95.1 %)</p> <p>Ratio = 24.1 (103.7 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.563-20.563 min, 1 scans) (**) Jan1418.D</p> <p>Lib Match Score=76.6</p> </div> </div>								

Quantitation Results Report (QT Reviewed)

Data File	Jan1419.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/14/2022 9:01:54 PM
Sample Name	14-Jan-22_ISTBLK_19	Instrument	GCMS
Vial	10	Multiplier	1.00
DA Method File		Comment	SVOC-8270-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011422 bna SIM 2.batch.bin	Last Calib Update	1/17/2022 8:49:06 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.509	152.0	213281	40.0000	ng/ml	0.013
M Naphthalene-d8	5.941	136.0	399778	40.0000	ng/ml	0.000
M Acenaphthene-d10	8.013	164.0	229587	40.0000	ng/ml	0.013
M Phenanthrene-d10	9.780	188.0	467279	40.0000	ng/ml	0.000
M Chrysene-d12	14.739	240.0	327147	40.0000	ng/ml	0.013
M Perylene-d12	18.512	264.0	260842	40.0000	ng/ml	0.013
System Monitoring Compounds						
S Nitrobenzene-d5	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = NA%		
S 2-Fluorobiphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = NA%		
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = NA%		
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.038	154.0	0		ng/ml md	1
T Fluorene	0.000		0	N.D.		
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.727	228.0	0		ng/ml md	1
T Chrysene	14.789	228.0	0		ng/ml md	1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.388	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Nitrobenzene-d5	N.D.	5.14	54.0	37.0	128.0	36.6




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.95	102.0	19.9	129.0	11.0



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.79	142.0	140.8	115.0	59.7




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	113.1	115.0	67.8




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
2-Fluorobiphenyl	N.D.	7.26	171.0	38.0




Compound	Conc.	Exp RT	QIon	Exp Ratio
Acenaphthylene	N.D.	7.83	153.0	12.8







Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene		0		0	153.0		82.1	152.6
					152.0		41.0	76.1







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Fluorene	N.D.	8.67	165.0	98.7	167.0	13.8



Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.73	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.79	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.5	30.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.23	138.0	28.9




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.30	279.0	25.1	139.0	24.1



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.56	138.0	28.0	277.0	23.3



Audit Trail report

Batch name and path: \\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\QuantResults\011422 bna SIM 2.batch.bin
Quant batch version: 10.0
Quant reporting version: 10.0

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdNewBatchTable	BL2000\jheine	1/17/2022 8:24:28 AM	Create new batch \\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\011422 bna SIM 2.batch.bin			✓	
CmdImportSamplesFromWorklist	BL2000\jheine	1/17/2022 8:25:21 AM	Add samples from worklist: \\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1419.D, \\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1418.D, \\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1417.D, \\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1416.D, \\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1415.D, \\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1414.D, \\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1413.D, \\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1412.D, \\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1411.D, \\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1410.D			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 8:26:17 AM	Set SampleType = TuneCheck for sample Jan1410.D; previous value = Sample			✓	
CmdStartMethodEditing	BL2000\jheine	1/17/2022 8:27:03 AM	Start method editing			✓	
CmdImportMethodFromBatch	BL2000\jheine	1/17/2022 8:27:04 AM	Import method from batch \\MASSHUNTER\Org\Data\SV5975.I\sh011322\2 e8270d bna SIM\011322 bna SIM 2.batch.bin			✓	
CmdApplyMethodToAllSamples	BL2000\jheine	1/17/2022 8:27:13 AM	Apply method to all samples			✓	
CmdMethodClear	BL2000\jheine	1/17/2022 8:27:13 AM	Clear method			✓	
CmdEndMethodEditing	BL2000\jheine	1/17/2022 8:27:13 AM	End method editing			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 8:27:20 AM	Set SampleType = Calibration for sample Jan1411.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 8:27:21 AM	Set SampleType = Calibration for sample Jan1412.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 8:27:25 AM	Set SampleType = Calibration for sample Jan1413.D; previous value = Sample			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 8:27:28 AM	Set SampleType = Calibration for sample Jan1414.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 8:27:30 AM	Set SampleType = Calibration for sample Jan1415.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 8:27:33 AM	Set SampleType = Calibration for sample Jan1416.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 8:27:35 AM	Set SampleType = Calibration for sample Jan1417.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 8:27:38 AM	Set SampleType = QC for sample Jan1418.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 8:27:42 AM	Set LevelName = ICV for sample Jan1418.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 8:27:44 AM	Set LevelName = 1 for sample Jan1417.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 8:27:48 AM	Set LevelName = 2 for sample Jan1416.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 8:27:50 AM	Set LevelName = 3 for sample Jan1415.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 8:27:54 AM	Set LevelName = 4 for sample Jan1414.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 8:28:00 AM	Set LevelName = 5 for sample Jan1413.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 8:28:03 AM	Set LevelName = 6 for sample Jan1412.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 8:28:06 AM	Set LevelName = 7 for sample Jan1411.D; previous value =			✓	
CmdQuantitate	BL2000\jheine	1/17/2022 8:28:11 AM	Quantitate all compounds in all samples			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/17/2022 8:29:14 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1413.D, from x, y = 5.941, 578 to 6.040, 84, result = 2700; previous integration is from x, y = 5.878, 82 to 6.040, 84 and previous response = 6815.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:29:16 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1413.D to y = 84, new integration is from x, y = 5.941, 84 to 6.040, 84 and new response = 4180; previous integration is from x, y = 5.941, 578 to 6.040, 84 and previous response = 2700.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/17/2022 8:29:34 AM	Manually integrate qualifier 153.0 of compound Acenaphthylene in sample Jan1413.D from x, y = 7.813, 1143 to 7.876, 2758; result = -4349			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/17/2022 8:29:36 AM	Snap baseline for qualifier 153.0 of compound Acenaphthylene in sample Jan1413.D from x = 7.813 to x = 7.876, new integration is from x, y = 7.813, 98 to 7.876, 167 and new response = 2448; previous integration is from x, y = 7.813, 1143 to 7.876, 2758 and previous response = -4349.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:29:37 AM	Drop baseline for qualifier 153.0 of compound Acenaphthylene in sample Jan1413.D to y = 98, new integration is from x, y = 7.813, 98 to 7.876, 98 and new response = 2577; previous integration is from x, y = 7.813, 98 to 7.876, 167 and previous response = 2448.			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	1/17/2022 8:29:46 AM	Split qualifier 167.0 of compound Fluorene in sample Jan1413.D and keep left peak, new integration is from x, y = 8.636, 70.0774603174603 to 8.798, 70.0774603174603 and new response = 2126, previous integration is from x, y = 8.636, 70 to 8.972, 70 and previous response = 5351.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 8:31:06 AM	Manually integrate compound Benzo(g,h,i)perylene in sample Jan1413.D, from x, y = 20.526, 924 to 20.674, 1449, result = 7107; previous integration is from x, y = 20.538, 651 to 20.621, 606 and previous response = 11242.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/17/2022 8:31:08 AM	Snap baseline for compound Benzo(g,h,i)perylene in sample Jan1413.D, from x = 20.526 to x = 20.674, new integration is from x, y = 20.526, 111 to 20.674, 267 and new response = 15982; previous integration is from x, y = 20.526, 924 to 20.674, 1449 and previous response = 7107.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:31:09 AM	Drop baseline for compound Benzo(g,h,i)perylene in sample Jan1413.D to y = 111, new integration is from x, y = 20.526, 111 to 20.674, 111 and new response = 16676; previous integration is from x, y = 20.526, 111 to 20.674, 267 and previous response = 15982.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:31:23 AM	Set UserAnnotation = BA for compound Benzo(g,h,i)perylene in sample Jan1413.D; previous value =			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdUpdateRetentionTimes	BL2000\jheine	1/17/2022 8:31:37 AM	Update retention time for compound Perylene-d12; Chrysene-d12; Phenanthrene-d10; Acenaphthene-d10; Naphthalene-d8; 1,4-Dichlorobenzene-d4; o-Terphenyl; Terphenyl-d14; 2-Fluorobiphenyl; Nitrobenzene-d5; Dibenzo(a,h)anthracene; Indeno(1,2,3-cd)pyrene; Benzo(a)pyrene; Benzo(k)fluoranthene; Benzo(b)fluoranthene; Chrysene; Benzo(a)Anthracene; Pyrene; Fluoranthene; Anthracene; Phenanthrene; Fluorene; Acenaphthene; Acenaphthylene; 1-Methylnaphthalene; 2-Methylnaphthalene; Naphthalene; Benzo(g,h,i)perylene;			✓	
CmdQuantitate	BL2000\jheine	1/17/2022 8:31:44 AM	Quantitate all compounds in all samples			✓	
CmdSaveBatchTable	BL2000\jheine	1/17/2022 8:32:15 AM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\QuantResults\011422 bna SIM 2.batch.bin			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdUpdateQualifierRatios	BL2000\jheine	1/17/2022 8:32:47 AM	Update qualifier ratios for compound Perylene-d12; Update qualifier ratios for compound Chrysene-d12; Update qualifier ratios for compound Phenanthrene-d10; Update qualifier ratios for compound Acenaphthene-d10; Update qualifier ratios for compound Naphthalene-d8; Update qualifier ratios for compound 1,4-Dichlorobenzene-d4; Update qualifier ratios for compound Terphenyl-d14; Update qualifier ratios for compound 2-Fluorobiphenyl; Update qualifier ratios for compound Nitrobenzene-d5; Update qualifier ratios for compound Benzo(g,h,i)perylene; Update qualifier ratios for compound Dibenzo(a,h)anthracene; Update qualifier ratios for compound Indeno(1,2,3-cd)pyrene; Update qualifier ratios for compound Benzo(a)pyrene; Update qualifier ratios for compound Benzo(k)fluoranthene; Update qualifier ratios for compound Benzo(b)fluoranthene; Update qualifier ratios for compound Chrysene; Update qualifier ratios for compound Benzo(a)Anthracene; Update qualifier ratios for compound Pyrene; Update qualifier ratios for compound Fluoranthene; Update qualifier ratios for compound Anthracene; Update qualifier ratios for compound Phenanthrene; Update qualifier ratios for compound Fluorene; Update qualifier ratios for compound Acenaphthene; Update qualifier ratios for compound Acenaphthylene; Update qualifier ratios for compound 1-Methylnaphthalene; Update qualifier ratios for compound 2-Methylnaphthalene; Update qualifier ratios for compound Naphthalene; Update qualifier ratios for compound o-Terphenyl;			✓	
CmdQuantitate	BL2000\jheine	1/17/2022 8:32:54 AM	Quantitate all compounds in all samples			✓	
CmdQuantitate	BL2000\jheine	1/17/2022 8:33:08 AM	Quantitate all compounds in all samples			✓	
CmdQuantitate	BL2000\jheine	1/17/2022 8:34:18 AM	Quantitate all compounds in all samples			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/17/2022 8:36:10 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1412.D, from x, y = 5.941, 821 to 6.041, 107, result = 6881; previous integration is from x, y = 5.909, 111 to 6.041, 107 and previous response = 11872.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:36:11 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1412.D to y = 107, new integration is from x, y = 5.941, 107 to 6.041, 107 and new response = 9021; previous integration is from x, y = 5.941, 821 to 6.041, 107 and previous response = 6881.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/17/2022 8:37:13 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1414.D, from x, y = 5.941, 1712 to 6.041, 1414, result = -6315; previous integration is from x, y = 5.906, 78 to 6.153, 78 and previous response = 5305.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/17/2022 8:37:17 AM	Snap baseline for qualifier 102.0 of compound Naphthalene in sample Jan1414.D from x = 5.941 to x = 6.041, new integration is from x, y = 5.941, 1393 to 6.041, 106 and new response = -1437; previous integration is from x, y = 5.941, 1712 to 6.041, 1414 and previous response = -6315.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:37:17 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1414.D to y = 106, new integration is from x, y = 5.941, 106 to 6.041, 106 and new response = 2421; previous integration is from x, y = 5.941, 1393 to 6.041, 106 and previous response = -1437.			✓	
CmdManuallyIntegrateApplyTargetRtToQualifier	BL2000\jheine	1/17/2022 8:37:29 AM	Apply target integration range 7.801-7.913 to qualifier 153.0 for compound Acenaphthylene in sample Jan1414.D, new integration is from x, y = 7.801, 66 to 7.913, 88 and new response = 1342; previously no peak.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/17/2022 8:38:17 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1415.D, from x, y = 5.941, 385 to 6.016, 71, result = 850; previous integration is from x, y = 5.895, 71 to 6.016, 71 and previous response = 4019.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:38:19 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1415.D to y = 71, new integration is from x, y = 5.941, 71 to 6.016, 71 and new response = 1556; previous integration is from x, y = 5.941, 385 to 6.016, 71 and previous response = 850.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 8:38:28 AM	Manually integrate compound 1-Methylnaphthalene in sample Jan1415.D, from x, y = 6.877, 266 to 7.052, 191, result = 1731; previous integration is from x, y = 6.765, 76 to 6.877, 76 and previous response = 2919.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/17/2022 8:38:30 AM	Snap baseline for compound 1-Methylnaphthalene in sample Jan1415.D, from x = 6.877 to x = 7.052, new integration is from x, y = 6.877, 151 to 7.052, 96 and new response = 2829; previous integration is from x, y = 6.877, 266 to 7.052, 191 and previous response = 1731.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:38:31 AM	Drop baseline for compound 1-Methylnaphthalene in sample Jan1415.D to y = 96, new integration is from x, y = 6.877, 96 to 7.052, 96 and new response = 3118; previous integration is from x, y = 6.877, 151 to 7.052, 96 and previous response = 2829.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:38:35 AM	Set UserAnnotation = NI for compound 1-Methylnaphthalene in sample Jan1415.D; previous value =			✓	
CmdManuallyIntegrateApplyTargetRtToQualifier	BL2000\jheine	1/17/2022 8:38:42 AM	Apply target integration range 7.802-7.988 to qualifier 153.0 for compound Acenaphthylene in sample Jan1415.D, new integration is from x, y = 7.802, 64 to 7.988, 73 and new response = 661; previously no peak.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/17/2022 8:39:27 AM	Manually integrate qualifier 129.0 of compound Naphthalene in sample Jan1416.D, from x, y = 5.910, 80 to 6.003, 102, result = 240; previous integration is from x, y = 5.910, 80 to 6.068, 80 and previous response = 324.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:39:28 AM	Drop baseline for qualifier 129.0 of compound Naphthalene in sample Jan1416.D to y = 80, new integration is from x, y = 5.910, 80 to 6.003, 80 and new response = 301; previous integration is from x, y = 5.910, 80 to 6.003, 102 and previous response = 240.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/17/2022 8:39:33 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1416.D, from x, y = 5.941, 1041 to 6.053, 914, result = -4869; previous integration is from x, y = 5.904, 69 to 6.091, 69 and previous response = 3561.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/17/2022 8:39:34 AM	Snap baseline for qualifier 102.0 of compound Naphthalene in sample Jan1416.D from x = 5.941 to x = 6.053, new integration is from x, y = 5.941, 1317 to 6.053, 93 and new response = -3030; previous integration is from x, y = 5.941, 1041 to 6.053, 914 and previous response = -4869.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:39:35 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1416.D to y = 93, new integration is from x, y = 5.941, 93 to 6.053, 93 and new response = 1097; previous integration is from x, y = 5.941, 1317 to 6.053, 93 and previous response = -3030.			✓	
CmdManuallyIntegrateApplyTargetRtToQualifier	BL2000\jheine	1/17/2022 8:39:45 AM	Apply target integration range 7.803-7.976 to qualifier 153.0 for compound Acenaphthylene in sample Jan1416.D, new integration is from x, y = 7.803, 63 to 7.976, 69 and new response = 257; previous integration is from x, y = 7.988, 64 to 8.125, 64 and previous response = 1612.			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	1/17/2022 8:39:50 AM	Split peak for compound Acenaphthene in sample Jan1416.D and keep right peak, new integration is from x, y = 7.963, 61.8891534391534 to 8.100, 61.8891534391534 and new response = 2240, previous integration is from x, y = 7.963, 62 to 8.100, 62 and previous response = 2240.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 8:39:55 AM	Manually integrate compound Acenaphthene in sample Jan1416.D, from x, y = 8.025, 115 to 8.100, 62, result = 1243; previous integration is from x, y = 7.963, 62 to 8.100, 62 and previous response = 2240.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:39:57 AM	Drop baseline for compound Acenaphthene in sample Jan1416.D to y = 62, new integration is from x, y = 8.025, 62 to 8.100, 62 and new response = 1362; previous integration is from x, y = 8.025, 115 to 8.100, 62 and previous response = 1243.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:39:59 AM	Set UserAnnotation = CO for compound Acenaphthene in sample Jan1416.D; previous value =			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateSplit	BL2000\jheine	1/17/2022 8:40:05 AM	Split peak for compound Phenanthrene in sample Jan1416.D and keep left peak, new integration is from x, y = 9.749, 66.7545695045695 to 9.842, 66.7545695045695 and new response = 2407, previous integration is from x, y = 9.749, 67 to 9.953, 67 and previous response = 4451.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:40:08 AM	Set UserAnnotation = CO for compound Phenanthrene in sample Jan1416.D; previous value =			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	1/17/2022 8:40:11 AM	Split peak for compound Anthracene in sample Jan1416.D and keep right peak, new integration is from x, y = 9.842, 66.7545695045695 to 9.953, 66.7545695045695 and new response = 2045, previous integration is from x, y = 9.749, 67 to 9.953, 67 and previous response = 4451.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:40:13 AM	Set UserAnnotation = CO for compound Anthracene in sample Jan1416.D; previous value =			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/17/2022 8:40:48 AM	Manually integrate qualifier 128.0 of compound Nitrobenzene-d5 in sample Jan1416.D, from x, y = 5.134, 112 to 5.230, 133, result = 98; previous integration is from x, y = 5.134, 112 to 5.317, 108 and previous response = 204.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:40:49 AM	Drop baseline for qualifier 128.0 of compound Nitrobenzene-d5 in sample Jan1416.D to y = 112, new integration is from x, y = 5.134, 112 to 5.230, 112 and new response = 160; previous integration is from x, y = 5.134, 112 to 5.230, 133 and previous response = 98.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/17/2022 8:41:25 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1417.D, from x, y = 5.953, 167 to 6.016, 69, result = 248; previous integration is from x, y = 5.905, 69 to 6.016, 69 and previous response = 3211.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:41:27 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1417.D to y = 69, new integration is from x, y = 5.953, 69 to 6.016, 69 and new response = 432; previous integration is from x, y = 5.953, 167 to 6.016, 69 and previous response = 248.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/17/2022 8:41:35 AM	Manually integrate qualifier 142.0 of compound 2-Methylnaphthalene in sample Jan1417.D from x, y = 6.765, 80 to 6.877, 88; result = 665			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:41:37 AM	Drop baseline for qualifier 142.0 of compound 2-Methylnaphthalene in sample Jan1417.D to y = 80, new integration is from x, y = 6.765, 80 to 6.877, 80 and new response = 691; previous integration is from x, y = 6.765, 80 to 6.877, 88 and previous response = 665.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/17/2022 8:41:47 AM	Manually integrate qualifier 153.0 of compound Acenaphthylene in sample Jan1417.D, from x, y = 7.814, 97 to 7.851, 176, result = -57; previous integration is from x, y = 8.025, 64 to 8.100, 64 and previous response = 787.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/17/2022 8:41:48 AM	Snap baseline for qualifier 153.0 of compound Acenaphthylene in sample Jan1417.D from x = 7.814 to x = 7.851, new integration is from x, y = 7.814, 62 to 7.851, 77 and new response = 93; previous integration is from x, y = 7.814, 97 to 7.851, 176 and previous response = -57.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:41:49 AM	Drop baseline for qualifier 153.0 of compound Acenaphthylene in sample Jan1417.D to y = 62, new integration is from x, y = 7.814, 62 to 7.851, 62 and new response = 110; previous integration is from x, y = 7.814, 62 to 7.851, 77 and previous response = 93.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 8:41:55 AM	Manually integrate compound Acenaphthene in sample Jan1417.D, from x, y = 8.025, 311 to 8.125, 389, result = -928; previous integration is from x, y = 7.966, 61 to 8.275, 61 and previous response = 1688.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/17/2022 8:41:56 AM	Snap baseline for compound Acenaphthene in sample Jan1417.D, from x = 8.025 to x = 8.125, new integration is from x, y = 8.025, 145 to 8.125, 70 and new response = 522; previous integration is from x, y = 8.025, 311 to 8.125, 389 and previous response = -928.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:41:57 AM	Drop baseline for compound Acenaphthene in sample Jan1417.D to y = 70, new integration is from x, y = 8.025, 70 to 8.125, 70 and new response = 747; previous integration is from x, y = 8.025, 145 to 8.125, 70 and previous response = 522.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSetTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:41:58 AM	Set UserAnnotation = CO for compound Acenaphthene in sample Jan1417.D; previous value =			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/17/2022 8:42:03 AM	Manually integrate qualifier 153.0 of compound Acenaphthene in sample Jan1417.D from x, y = 8.025, 139 to 8.100, 167; result = 384			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/17/2022 8:42:05 AM	Snap baseline for qualifier 153.0 of compound Acenaphthene in sample Jan1417.D from x = 8.025 to x = 8.100, new integration is from x, y = 8.025, 97 to 8.100, 75 and new response = 686; previous integration is from x, y = 8.025, 139 to 8.100, 167 and previous response = 384.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:42:05 AM	Drop baseline for qualifier 153.0 of compound Acenaphthene in sample Jan1417.D to y = 75, new integration is from x, y = 8.025, 75 to 8.100, 75 and new response = 736; previous integration is from x, y = 8.025, 97 to 8.100, 75 and previous response = 686.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 8:42:17 AM	Manually integrate compound Fluoranthene in sample Jan1417.D from x, y = 11.398, 69 to 11.547, 151; result = 756			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/17/2022 8:42:19 AM	Snap baseline for compound Fluoranthene in sample Jan1417.D, from x = 11.398 to x = 11.547, new integration is from x, y = 11.398, 58 to 11.547, 69 and new response = 1173; previous integration is from x, y = 11.398, 69 to 11.547, 151 and previous response = 756.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:42:20 AM	Drop baseline for compound Fluoranthene in sample Jan1417.D to y = 58, new integration is from x, y = 11.398, 58 to 11.547, 58 and new response = 1222; previous integration is from x, y = 11.398, 58 to 11.547, 69 and previous response = 1173.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 8:43:14 AM	Manually integrate compound Pyrene in sample Jan1417.D from x, y = 11.769, 97 to 11.905, 181; result = 678			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/17/2022 8:43:16 AM	Snap baseline for compound Pyrene in sample Jan1417.D, from x = 11.769 to x = 11.905, new integration is from x, y = 11.769, 63 to 11.905, 78 and new response = 1239; previous integration is from x, y = 11.769, 97 to 11.905, 181 and previous response = 678.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:43:16 AM	Drop baseline for compound Pyrene in sample Jan1417.D to y = 63, new integration is from x, y = 11.769, 63 to 11.905, 63 and new response = 1300; previous integration is from x, y = 11.769, 63 to 11.905, 78 and previous response = 1239.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/17/2022 8:43:21 AM	Manually integrate qualifier 101.0 of compound Pyrene in sample Jan1417.D, from x, y = 11.747, 60 to 11.868, 73, result = 142; previous integration is from x, y = 11.747, 60 to 11.917, 60 and previous response = 209.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:43:22 AM	Drop baseline for qualifier 101.0 of compound Pyrene in sample Jan1417.D to y = 60, new integration is from x, y = 11.747, 60 to 11.868, 60 and new response = 189; previous integration is from x, y = 11.747, 60 to 11.868, 73 and previous response = 142.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 8:43:29 AM	Manually integrate compound Benzo(a)Anthracene in sample Jan1417.D from x, y = 14.652, 51 to 14.764, 94; result = 1717			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:43:30 AM	Drop baseline for compound Benzo(a)Anthracene in sample Jan1417.D to y = 51, new integration is from x, y = 14.652, 51 to 14.764, 51 and new response = 1860; previous integration is from x, y = 14.652, 51 to 14.764, 94 and previous response = 1717.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:43:32 AM	Set UserAnnotation = NI for compound Benzo(a)Anthracene in sample Jan1417.D; previous value =			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdClearManualIntegration	BL2000\jheine	1/17/2022 8:43:36 AM	Clear manual integration of target signal for compound Pyrene in sample Jan1417.D				Agilent.MassSpectrometry.DataAnalysis.Quantitative.ApplicationCommandException: Integrator did not find any peaks at Agilent.MassSpectrometry.DataAnalysis.Quantitative.Analysis.MeasuredIon.ClearManualIntegration() at Agilent.MassSpectrometry.DataAnalysis.Quantitative.CmdClearManualIntegration.Do() at Agilent.MassSpectrometry.CommandModel.CommandHistory.Invoke(ICommand cmd) at Agilent.MassSpectrometry.DataAnalysis.Quantitative.AppCommandContext._Invoke(ICommand cmd)
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 8:43:42 AM	Manually integrate compound Pyrene in sample Jan1417.D from x, y = 11.769, 63 to 11.917, 75; result = 1256			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:43:43 AM	Drop baseline for compound Pyrene in sample Jan1417.D to y = 63, new integration is from x, y = 11.769, 63 to 11.917, 63 and new response = 1310; previous integration is from x, y = 11.769, 63 to 11.917, 75 and previous response = 1256.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:43:44 AM	Set UserAnnotation = NI for compound Pyrene in sample Jan1417.D; previous value =			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:43:49 AM	Set UserAnnotation = NI for compound Fluoranthene in sample Jan1417.D; previous value =			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 8:43:56 AM	Manually integrate compound Chrysene in sample Jan1417.D, from x, y = 14.764, 244 to 14.926, 169, result = -199; previous integration is from x, y = 14.659, 57 to 14.764, 58 and previous response = 1819.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/17/2022 8:43:57 AM	Snap baseline for compound Chrysene in sample Jan1417.D, from x = 14.764 to x = 14.926, new integration is from x, y = 14.764, 161 to 14.926, 65 and new response = 706; previous integration is from x, y = 14.764, 244 to 14.926, 169 and previous response = -199.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:43:58 AM	Drop baseline for compound Chrysene in sample Jan1417.D to y = 65, new integration is from x, y = 14.764, 65 to 14.926, 65 and new response = 1172; previous integration is from x, y = 14.764, 161 to 14.926, 65 and previous response = 706.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/17/2022 8:44:02 AM	Manually integrate qualifier 226.0 of compound Chrysene in sample Jan1417.D from x, y = 14.751, 98 to 14.938, 75; result = 56			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/17/2022 8:44:04 AM	Snap baseline for qualifier 226.0 of compound Chrysene in sample Jan1417.D from x = 14.751 to x = 14.938, new integration is from x, y = 14.751, 85 to 14.938, 58 and new response = 222; previous integration is from x, y = 14.751, 98 to 14.938, 75 and previous response = 56.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:44:04 AM	Drop baseline for qualifier 226.0 of compound Chrysene in sample Jan1417.D to y = 58, new integration is from x, y = 14.751, 58 to 14.938, 58 and new response = 373; previous integration is from x, y = 14.751, 85 to 14.938, 58 and previous response = 222.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/17/2022 8:44:10 AM	Manually integrate qualifier 229.0 of compound Chrysene in sample Jan1417.D from x, y = 14.764, 123 to 14.888, 111; result = -146			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/17/2022 8:44:11 AM	Snap baseline for qualifier 229.0 of compound Chrysene in sample Jan1417.D from x = 14.764 to x = 14.888, new integration is from x, y = 14.764, 93 to 14.888, 62 and new response = 147; previous integration is from x, y = 14.764, 123 to 14.888, 111 and previous response = -146.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:44:12 AM	Drop baseline for qualifier 229.0 of compound Chrysene in sample Jan1417.D to y = 62, new integration is from x, y = 14.764, 62 to 14.888, 62 and new response = 262; previous integration is from x, y = 14.764, 93 to 14.888, 62 and previous response = 147.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:44:20 AM	Set UserAnnotation = NI for compound Chrysene in sample Jan1417.D; previous value =			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 8:44:29 AM	Manually integrate compound Benzo(k)fluoranthene in sample Jan1417.D from x, y = 17.783, 190 to 17.919, 123; result = 68			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/17/2022 8:44:30 AM	Snap baseline for compound Benzo(k)fluoranthene in sample Jan1417.D, from x = 17.783 to x = 17.919, new integration is from x, y = 17.783, 159 to 17.919, 70 and new response = 410; previous integration is from x, y = 17.783, 190 to 17.919, 123 and previous response = 68.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:44:30 AM	Drop baseline for compound Benzo(k)fluoranthene in sample Jan1417.D to y = 70, new integration is from x, y = 17.783, 70 to 17.919, 70 and new response = 773; previous integration is from x, y = 17.783, 159 to 17.919, 70 and previous response = 410.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/17/2022 8:44:34 AM	Manually integrate qualifier 253.0 of compound Benzo(k)fluoranthene in sample Jan1417.D from x, y = 17.783, 87 to 17.869, 87; result = 29			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/17/2022 8:44:36 AM	Snap baseline for qualifier 253.0 of compound Benzo(k)fluoranthene in sample Jan1417.D from x = 17.783 to x = 17.869, new integration is from x, y = 17.783, 84 to 17.869, 64 and new response = 97; previous integration is from x, y = 17.783, 87 to 17.869, 87 and previous response = 29.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:44:37 AM	Drop baseline for qualifier 253.0 of compound Benzo(k)fluoranthene in sample Jan1417.D to y = 64, new integration is from x, y = 17.783, 64 to 17.869, 64 and new response = 149; previous integration is from x, y = 17.783, 84 to 17.869, 64 and previous response = 97.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 8:44:44 AM	Manually integrate compound Benzo(a)pyrene in sample Jan1417.D, from x, y = 18.351, 108 to 18.462, 162, result = 76; previous integration is from x, y = 18.462, 62 to 18.586, 62 and previous response = 933.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/17/2022 8:44:45 AM	Snap baseline for compound Benzo(a)pyrene in sample Jan1417.D, from x = 18.351 to x = 18.462, new integration is from x, y = 18.351, 61 to 18.462, 74 and new response = 528; previous integration is from x, y = 18.351, 108 to 18.462, 162 and previous response = 76.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:44:46 AM	Drop baseline for compound Benzo(a)pyrene in sample Jan1417.D to y = 61, new integration is from x, y = 18.351, 61 to 18.462, 61 and new response = 571; previous integration is from x, y = 18.351, 61 to 18.462, 74 and previous response = 528.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:44:47 AM	Set UserAnnotation = NI for compound Benzo(a)pyrene in sample Jan1417.D; previous value =			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/17/2022 8:44:51 AM	Manually integrate qualifier253.0 of compound Benzo(a)pyrene in sample Jan1417.D from x, y = 18.351, 72 to 18.450, 102; result = -28			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/17/2022 8:44:53 AM	Snap baseline for qualifier 253.0 of compound Benzo(a)pyrene in sample Jan1417.D from x = 18.351 to x = 18.450, new integration is from x, y = 18.351, 63 to 18.450, 64 and new response = 112; previous integration is from x, y = 18.351, 72 to 18.450, 102 and previous response = -28.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:44:53 AM	Drop baseline for qualifier 253.0 of compound Benzo(a)pyrene in sample Jan1417.D to y = 63, new integration is from x, y = 18.351, 63 to 18.450, 63 and new response = 115; previous integration is from x, y = 18.351, 63 to 18.450, 64 and previous response = 112.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/17/2022 8:45:02 AM	Manually integrate qualifier279.0 of compound Dibenzo(a,h)anthracene in sample Jan1417.D from x, y = 20.266, 64 to 20.414, 63; result = 172			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:45:04 AM	Drop baseline for qualifier 279.0 of compound Dibenzo(a,h)anthracene in sample Jan1417.D to y = 63, new integration is from x, y = 20.266, 63 to 20.414, 63 and new response = 176; previous integration is from x, y = 20.266, 64 to 20.414, 63 and previous response = 172.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 8:45:12 AM	Manually integrate compound Benzo(g,h,i)perylene in sample Jan1417.D from x, y = 20.538, 59 to 20.662, 127; result = 555			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/17/2022 8:45:14 AM	Snap baseline for compound Benzo(g,h,i)perylene in sample Jan1417.D, from x = 20.538 to x = 20.662, new integration is from x, y = 20.538, 59 to 20.662, 73 and new response = 755; previous integration is from x, y = 20.538, 59 to 20.662, 127 and previous response = 555.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:45:14 AM	Drop baseline for compound Benzo(g,h,i)perylene in sample Jan1417.D to y = 59, new integration is from x, y = 20.538, 59 to 20.662, 59 and new response = 807; previous integration is from x, y = 20.538, 59 to 20.662, 73 and previous response = 755.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:45:16 AM	Set UserAnnotation = NI for compound Benzo(g,h,i)perylene in sample Jan1417.D; previous value =			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/17/2022 8:45:22 AM	Manually integrate qualifier 277.0 of compound Benzo(g,h,i)perylene in sample Jan1417.D from x, y = 20.526, 56 to 20.637, 60; result = 192			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:45:23 AM	Drop baseline for qualifier 277.0 of compound Benzo(g,h,i)perylene in sample Jan1417.D to y = 56, new integration is from x, y = 20.526, 56 to 20.637, 56 and new response = 205; previous integration is from x, y = 20.526, 56 to 20.637, 60 and previous response = 192.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 8:45:31 AM	Manually integrate compound Nitrobenzene-d5 in sample Jan1417.D from x, y = 5.118, 270 to 5.255, 276; result = 260			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:45:32 AM	Drop baseline for compound Nitrobenzene-d5 in sample Jan1417.D to y = 270, new integration is from x, y = 5.118, 270 to 5.255, 270 and new response = 285; previous integration is from x, y = 5.118, 270 to 5.255, 276 and previous response = 260.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:45:35 AM	Set UserAnnotation = NI for compound Nitrobenzene-d5 in sample Jan1417.D; previous value =			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/17/2022 8:45:39 AM	Manually integrate qualifier 54.0 of compound Nitrobenzene-d5 in sample Jan1417.D, from x, y = 5.118, 89 to 5.230, 90, result = 72; previous integration is from x, y = 5.131, 91 to 5.367, 83 and previous response = 118.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:45:41 AM	Drop baseline for qualifier 54.0 of compound Nitrobenzene-d5 in sample Jan1417.D to y = 89, new integration is from x, y = 5.118, 89 to 5.230, 89 and new response = 75; previous integration is from x, y = 5.118, 89 to 5.230, 90 and previous response = 72.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/17/2022 8:45:44 AM	Manually integrate qualifier 128.0 of compound Nitrobenzene-d5 in sample Jan1417.D from x, y = 5.131, 108 to 5.205, 109; result = 59			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:45:45 AM	Drop baseline for qualifier 128.0 of compound Nitrobenzene-d5 in sample Jan1417.D to y = 108, new integration is from x, y = 5.131, 108 to 5.205, 108 and new response = 61; previous integration is from x, y = 5.131, 108 to 5.205, 109 and previous response = 59.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 8:46:12 AM	Manually integrate compound 2-Fluorobiphenyl in sample Jan1417.D from x, y = 7.227, 52 to 7.352, 71; result = 789			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:46:14 AM	Drop baseline for compound 2-Fluorobiphenyl in sample Jan1417.D to y = 52, new integration is from x, y = 7.227, 52 to 7.352, 52 and new response = 861; previous integration is from x, y = 7.227, 52 to 7.352, 71 and previous response = 789.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/17/2022 8:46:19 AM	Manually integrate qualifier 171.0 of compound 2-Fluorobiphenyl in sample Jan1417.D from x, y = 7.239, 54 to 7.364, 55; result = 326			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:46:20 AM	Drop baseline for qualifier 171.0 of compound 2-Fluorobiphenyl in sample Jan1417.D to y = 54, new integration is from x, y = 7.239, 54 to 7.364, 54 and new response = 329; previous integration is from x, y = 7.239, 54 to 7.364, 55 and previous response = 326.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:46:22 AM	Set UserAnnotation = NI for compound 2-Fluorobiphenyl in sample Jan1417.D; previous value =			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 8:46:30 AM	Manually integrate compound o-Terphenyl in sample Jan1417.D from x, y = 10.274, 53 to 10.398, 55; result = 608			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:46:32 AM	Drop baseline for compound o-Terphenyl in sample Jan1417.D to y = 53, new integration is from x, y = 10.274, 53 to 10.398, 53 and new response = 615; previous integration is from x, y = 10.274, 53 to 10.398, 55 and previous response = 608.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/17/2022 8:46:37 AM	Manually integrate qualifier 229.0 of compound o-Terphenyl in sample Jan1417.D from x, y = 10.287, 55 to 10.385, 57; result = 396			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:46:38 AM	Drop baseline for qualifier 229.0 of compound o-Terphenyl in sample Jan1417.D to y = 55, new integration is from x, y = 10.287, 55 to 10.385, 55 and new response = 402; previous integration is from x, y = 10.287, 55 to 10.385, 57 and previous response = 396.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/17/2022 8:46:42 AM	Manually integrate qualifier 215.0 of compound o-Terphenyl in sample Jan1417.D from x, y = 10.287, 55 to 10.385, 55; result = 270			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:46:45 AM	Drop baseline for qualifier 215.0 of compound o-Terphenyl in sample Jan1417.D to y = 55, new integration is from x, y = 10.287, 55 to 10.385, 55 and new response = 270; previous integration is from x, y = 10.287, 55 to 10.385, 55 and previous response = 270.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/17/2022 8:47:48 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1418.D, from x, y = 5.941, 467 to 6.041, 73, result = 3713; previous integration is from x, y = 5.903, 73 to 6.041, 73 and previous response = 7853.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:47:50 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1418.D to y = 73, new integration is from x, y = 5.941, 73 to 6.041, 73 and new response = 4894; previous integration is from x, y = 5.941, 467 to 6.041, 73 and previous response = 3713.			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	1/17/2022 8:47:55 AM	Split peak for compound 2-Methylnaphthalene in sample Jan1418.D and keep left peak, new integration is from x, y = 6.765, 76.8791208791209 to 6.877, 76.8791208791209 and new response = 15117, previous integration is from x, y = 6.765, 77 to 7.052, 77 and previous response = 30147.			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	1/17/2022 8:48:02 AM	Split peak for compound 1-Methylnaphthalene in sample Jan1418.D and keep right peak, new integration is from x, y = 6.877, 76.8791208791209 to 7.052, 76.8791208791209 and new response = 15029, previous integration is from x, y = 6.765, 77 to 7.052, 77 and previous response = 30147.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateSplit	BL2000\jheine	1/17/2022 8:48:05 AM	Split peak for compound 1-Methylnaphthalene in sample Jan1418.D and keep left peak, new integration is from x, y = 6.877, 76.8791208791209 to 6.952, 76.8791208791209 and new response = 13812, previous integration is from x, y = 6.877, 77 to 7.052, 77 and previous response = 15029.			✓	
CmdManuallyIntegrateApplyTargetRtToQualifier	BL2000\jheine	1/17/2022 8:48:19 AM	Apply target integration range 7.801-7.913 to qualifier 153.0 for compound Acenaphthylene in sample Jan1418.D, new integration is from x, y = 7.801, 65 to 7.913, 123 and new response = 3000; previously no peak.			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	1/17/2022 8:48:29 AM	Split qualifier 167.0 of compound Fluorene in sample Jan1418.D and keep left peak, new integration is from x, y = 8.640, 67.2631944444444 to 8.786, 67.2631944444444 and new response = 2554, previous integration is from x, y = 8.640, 67 to 8.973, 67 and previous response = 6527.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdCalibrate	BL2000\jheine	1/17/2022 8:49:06 AM	Replace level ICV with QC sample Jan1418.D for compounds {Benzo(g,h,i)perylene, Dibenzo(a,h)anthracene, Indeno(1,2,3-cd)pyrene, Benzo(a)pyrene, Benzo(k)fluoranthene, Benzo(b)fluoranthene, Chrysene, Benzo(a)Anthracene, Terphenyl-d14, Pyrene, Fluoranthene, Anthracene, Phenanthrene, Fluorene, Acenaphthene, Acenaphthylene, 2-Fluorobiphenyl, 1-Methylnaphthalene, 2-Methylnaphthalene, Naphthalene, Nitrobenzene-d5, o-Terphenyl}; Replace level 1 with Calibration sample Jan1417.D for compounds {Benzo(g,h,i)perylene, Dibenzo(a,h)anthracene, Indeno(1,2,3-cd)pyrene, Benzo(a)pyrene, Benzo(k)fluoranthene, Benzo(b)fluoranthene, Chrysene, Benzo(a)Anthracene, Terphenyl-d14, Pyrene, Fluoranthene, Anthracene, Phenanthrene, Fluorene, Acenaphthene, Acenaphthylene, 2-Fluorobiphenyl, 1-Methylnaphthalene, 2-Methylnaphthalene, Naphthalene, Nitrobenzene-d5, o-Terphenyl}; Replace level 2 with Calibration sample Jan1416.D for compounds {Benzo(g,h,i)perylene, Dibenzo(a,h)anthracene, Indeno(1,2,3-cd)pyrene, Benzo(a)pyrene, Benzo(k)fluoranthene, Benzo(b)fluoranthene, Chrysene, Benzo(a)Anthracene, Terphenyl-d14, Pyrene, Fluoranthene, Anthracene, Phenanthrene, Fluorene, Acenaphthene, Acenaphthylene, 2-Fluorobiphenyl, 1-Methylnaphthalene, 2-Methylnaphthalene, Naphthalene, Nitrobenzene-d5, o-Terphenyl}; Replace level 3 with Calibration sample Jan1415.D for compounds {Benzo(g,h,i)perylene, Dibenzo(a,h)anthracene, Indeno(1,2,3-cd)pyrene, Benzo(a)pyrene, Benzo(k)fluoranthene, Benzo(b)fluoranthene, Chrysene, Benzo(a)Anthracene, Terphenyl-d14, Pyrene, Fluoranthene, Anthracene, Phenanthrene, Fluorene, Acenaphthene, Acenaphthylene, 2-Fluorobiphenyl, 1-Methylnaphthalene, 2-Methylnaphthalene, Naphthalene, Nitrobenzene-d5, o-Terphenyl};			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
			<p>Nitrobenzene-d5, o-Terphenyl}; Replace level 4 with Calibration sample Jan1414.D for compounds {Benzo(g,h,i)perylene, Dibenzo(a,h)anthracene, Indeno(1,2,3-cd)pyrene, Benzo(a)pyrene, Benzo(k)fluoranthene, Benzo(b)fluoranthene, Chrysene, Benzo(a)Anthracene, Terphenyl-d14, Pyrene, Fluoranthene, Anthracene, Phenanthrene, Fluorene, Acenaphthene, Acenaphthylene, 2-Fluorobiphenyl, 1-Methylnaphthalene, 2-Methylnaphthalene, Naphthalene, Nitrobenzene-d5, o-Terphenyl}; Replace level 5 with Calibration sample Jan1413.D for compounds {Benzo(g,h,i)perylene, Dibenzo(a,h)anthracene, Indeno(1,2,3-cd)pyrene, Benzo(a)pyrene, Benzo(k)fluoranthene, Benzo(b)fluoranthene, Chrysene, Benzo(a)Anthracene, Terphenyl-d14, Pyrene, Fluoranthene, Anthracene, Phenanthrene, Fluorene, Acenaphthene, Acenaphthylene, 2-Fluorobiphenyl, 1-Methylnaphthalene, 2-Methylnaphthalene, Naphthalene, Nitrobenzene-d5, o-Terphenyl}; Replace level 6 with Calibration sample Jan1412.D for compounds {Benzo(g,h,i)perylene, Dibenzo(a,h)anthracene, Indeno(1,2,3-cd)pyrene, Benzo(a)pyrene, Benzo(k)fluoranthene, Benzo(b)fluoranthene, Chrysene, Benzo(a)Anthracene, Terphenyl-d14, Pyrene, Fluoranthene, Anthracene, Phenanthrene, Fluorene, Acenaphthene, Acenaphthylene, 2-Fluorobiphenyl, 1-Methylnaphthalene, 2-Methylnaphthalene, Naphthalene, Nitrobenzene-d5, o-Terphenyl}; Replace level 7 with Calibration sample Jan1411.D for compounds {Benzo(g,h,i)perylene, Dibenzo(a,h)anthracene, Indeno(1,2,3-cd)pyrene, Benzo(a)pyrene, Benzo(k)fluoranthene, Benzo(b)fluoranthene, Chrysene, Benzo(a)Anthracene, Terphenyl-d14, Pyrene, Fluoranthene, Anthracene, Phenanthrene, Fluorene, Acenaphthene, Acenaphthylene, 2-Fluorobiphenyl, 1-Methylnaphthalene,</p>				

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
			2-Methylnaphthalene, Naphthalene, Nitrobenzene-d5, o-Terphenyl};				
CmdQuantitate	BL2000\jheine	1/17/2022 8:49:13 AM	Quantitate all compounds in all samples			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:50:32 AM	Set CurveFitWeight = weightOneOverX for compound Phenanthrene in all samples; previous value = weightOneOverXSquared			✓	
CmdQuantitate	BL2000\jheine	1/17/2022 8:50:38 AM	Quantitate all compounds in all samples			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:51:03 AM	Set CurveFitWeight = weightOneOverX for compound Benzo(a)Anthracene in all samples; previous value = weightOneOverXSquared			✓	
CmdQuantitate	BL2000\jheine	1/17/2022 8:51:08 AM	Quantitate all compounds in all samples			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:51:19 AM	Set CurveFitOrigin = originIgnore for compound Chrysene in all samples; previous value = originInclude			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:51:22 AM	Set CurveFit = fitAverageOfResponseFactors for compound Chrysene in all samples; previous value = fitQuadratic			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:51:25 AM	Set CurveFitWeight = weightEqual for compound Chrysene in all samples; previous value = weightOneOverXSquared			✓	
CmdQuantitate	BL2000\jheine	1/17/2022 8:51:31 AM	Quantitate all compounds in all samples			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:51:43 AM	Set CurveFit = fitQuadratic for compound Terphenyl-d14 in all samples; previous value = fitAverageOfResponseFactors			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:51:44 AM	Set CurveFitOrigin = originInclude for compound Terphenyl-d14 in all samples; previous value = originIgnore			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:51:45 AM	Set CurveFitWeight = weightOneOverX for compound Terphenyl-d14 in all samples; previous value = weightEqual			✓	
CmdQuantitate	BL2000\jheine	1/17/2022 8:51:50 AM	Quantitate all compounds in all samples			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:52:31 AM	Set CurveFit = fitQuadratic for compound Indeno(1,2,3-cd)pyrene in all samples; previous value = fitAverageOfResponseFactors			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:52:36 AM	Set CurveFitWeight = weightOneOverX for compound Indeno(1,2,3-cd)pyrene in all samples; previous value = weightEqual			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdQuantitate	BL2000\jheine	1/17/2022 8:52:41 AM	Quantitate all compounds in all samples			✓	
CmdSaveBatchTable	BL2000\jheine	1/17/2022 8:53:08 AM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011422\2 e8270c bna SIM\QuantResults\011422 bna SIM 2.batch.bin			✓	
CmdSaveBatchTable	BL2000\jheine	1/17/2022 8:53:30 AM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011422\2 e8270c bna SIM\QuantResults\011422 bna SIM 2.batch.bin			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 8:53:53 AM	Manually integrate compound Benzo(a)pyrene in sample Jan1419.D, from x, y = 18.363, 89 to 18.413, 182, result = -172; previous integration is from x, y = 18.463, 60 to 18.648, 61 and previous response = 1517.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/17/2022 8:53:55 AM	Snap baseline for compound Benzo(a)pyrene in sample Jan1419.D, from x = 18.363 to x = 18.413, new integration is from x, y = 18.363, 56 to 18.413, 64 and new response = 52; previous integration is from x, y = 18.363, 89 to 18.413, 182 and previous response = -172.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:53:56 AM	Drop baseline for compound Benzo(a)pyrene in sample Jan1419.D to y = 56, new integration is from x, y = 18.363, 56 to 18.413, 56 and new response = 64; previous integration is from x, y = 18.363, 56 to 18.413, 64 and previous response = 52.			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 8:53:58 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1419.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 8:54:03 AM	Manually integrate compound Acenaphthene in sample Jan1419.D, from x, y = 8.026, 97 to 8.150, 61, result = 113; previous integration is from x, y = 7.976, 61 to 8.150, 61 and previous response = 1385.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:54:05 AM	Drop baseline for compound Acenaphthene in sample Jan1419.D to y = 61, new integration is from x, y = 8.026, 61 to 8.150, 61 and new response = 250; previous integration is from x, y = 8.026, 97 to 8.150, 61 and previous response = 113.			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 8:54:06 AM	Zero out primary peak of compound Acenaphthene in sample Jan1419.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 8:54:13 AM	Manually integrate compound Chrysene in sample Jan1419.D, from x, y = 14.776, 110 to 14.876, 51, result = 63; previous integration is from x, y = 14.656, 50 to 14.876, 51 and previous response = 1799.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:54:14 AM	Drop baseline for compound Chrysene in sample Jan1419.D to y = 51, new integration is from x, y = 14.776, 51 to 14.876, 51 and new response = 240; previous integration is from x, y = 14.776, 110 to 14.876, 51 and previous response = 63.			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 8:54:16 AM	Zero out primary peak of compound Chrysene in sample Jan1419.D			✓	
CmdStartMethodEditing	BL2000\jheine	1/17/2022 8:54:22 AM	Start method editing			✓	
CmdImportMethodFromSample	BL2000\jheine	1/17/2022 8:54:22 AM	Import method from sample Jan1419.D			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:39 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:39 AM	Set PeakFilterThresholdValue = 556.047048741229 for compound Naphthalene; previous value = 1037.63454930473			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:39 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:40 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:40 AM	Set PeakFilterThresholdValue = 61.1233050731016 for qualifier 129.0 of compound Naphthalene; previous value = 112.174329251956			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:40 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:40 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:40 AM	Set PeakFilterThresholdValue = 110.383348557415 for qualifier 102.0 of compound Naphthalene; previous value = 161.337722202857			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:41 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:41 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:41 AM	Set PeakFilterThresholdValue = 308.667237500002 for compound 2-Methylnaphthalene; previous value = 588.19625396825			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:41 AM	No parameter change for ThresholdNumberOfPeaks			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:41 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:41 AM	Set PeakFilterThresholdValue = 434.502679515188 for qualifier 142.0 of compound 2-Methylnaphthalene; previous value = 867.611723242636			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:41 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:42 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:42 AM	Set PeakFilterThresholdValue = 184.261213073991 for qualifier 115.0 of compound 2-Methylnaphthalene; previous value = 308.814817007921			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:42 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:42 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:42 AM	Set PeakFilterThresholdValue = 349.881033854167 for compound 1-Methylnaphthalene; previous value = 595.299928571425			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:42 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:42 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:43 AM	Set PeakFilterThresholdValue = 395.844520979499 for qualifier 142.0 of compound 1-Methylnaphthalene; previous value = 662.394921309491			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:43 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:43 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:43 AM	Set PeakFilterThresholdValue = 237.381833068489 for qualifier 115.0 of compound 1-Methylnaphthalene; previous value = 377.588666044884			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:43 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:44 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:44 AM	Set PeakFilterThresholdValue = 537.083925833335 for compound Acenaphthylene; previous value = 977.574997222228			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:44 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:44 AM	No parameter change for PeakFilterThreshold			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:44 AM	Set PeakFilterThresholdValue = 68.7873861965026 for qualifier 153.0 of compound Acenaphthylene; previous value = 142.297492641816			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:44 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:45 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:45 AM	Set PeakFilterThresholdValue = 373.252000000011 for compound Acenaphthene; previous value = 702.823942203903			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:45 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:45 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:45 AM	Set PeakFilterThresholdValue = 218.562419571157 for qualifier 152.0 of compound Acenaphthene; previous value = 385.842848130719			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:45 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:46 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:46 AM	Set PeakFilterThresholdValue = 438.027552091583 for qualifier 153.0 of compound Acenaphthene; previous value = 806.667572980904			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:46 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:46 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:46 AM	Set PeakFilterThresholdValue = 424.777029134499 for compound Fluorene; previous value = 756.80948412701			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:46 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:46 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:47 AM	Set PeakFilterThresholdValue = 419.107271211773 for qualifier 165.0 of compound Fluorene; previous value = 729.532248155729			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:47 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:47 AM	No parameter change for PeakFilterThreshold			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:47 AM	Set PeakFilterThresholdValue = 58.8152577920192 for qualifier 167.0 of compound Fluorene; previous value = 85.20871582856			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:47 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:48 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:48 AM	Set PeakFilterThresholdValue = 694.128737567089 for compound Phenanthrene; previous value = 1378.20817410716			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:48 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:48 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:48 AM	Set PeakFilterThresholdValue = 107.4326524611 for qualifier 176.0 of compound Phenanthrene; previous value = 213.984541449823			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:48 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:49 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:49 AM	Set PeakFilterThresholdValue = 549.674737099558 for compound Anthracene; previous value = 1070.77109548611			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:49 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:49 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:49 AM	Set PeakFilterThresholdValue = 99.4845614153201 for qualifier 176.0 of compound Anthracene; previous value = 178.157498643721			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:49 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:50 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:50 AM	Set PeakFilterThresholdValue = 610.793500000007 for compound Fluoranthene; previous value = 1280.26819717778			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:50 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:50 AM	No parameter change for PeakFilterThreshold			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:50 AM	Set PeakFilterThresholdValue = 84.1386311384159 for qualifier 101.0 of compound Fluoranthene; previous value = 146.018350606525			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:50 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:51 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:51 AM	Set PeakFilterThresholdValue = 654.831749999997 for compound Pyrene; previous value = 1463.19161579774			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:51 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:51 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:51 AM	Set PeakFilterThresholdValue = 100.500391321538 for qualifier 101.0 of compound Pyrene; previous value = 203.253032152133			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:52 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:52 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:52 AM	Set PeakFilterThresholdValue = 930.104750000004 for compound Benzo(a)Anthracene; previous value = 1853.37234592252			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:52 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:52 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:52 AM	Set PeakFilterThresholdValue = 214.084265757749 for qualifier 229.0 of compound Benzo(a)Anthracene; previous value = 436.107213370423			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:53 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:53 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:53 AM	Set PeakFilterThresholdValue = 251.471683618724 for qualifier 226.0 of compound Benzo(a)Anthracene; previous value = 517.609002259047			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:53 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:53 AM	No parameter change for PeakFilterThreshold			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:54 AM	Set PeakFilterThresholdValue = 585.823999999995 for compound Chrysene; previous value = 1409.75245176248			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:54 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:54 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:54 AM	Set PeakFilterThresholdValue = 177.55192908342 for qualifier 226.0 of compound Chrysene; previous value = 446.502448884273			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:54 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:54 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:55 AM	Set PeakFilterThresholdValue = 125.316635310255 for qualifier 229.0 of compound Chrysene; previous value = 313.124961416453			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:55 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:55 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:55 AM	Set PeakFilterThresholdValue = 377.169306815265 for compound Benzo(b)fluoranthene; previous value = 696.285772650434			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:55 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:56 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:56 AM	Set PeakFilterThresholdValue = 85.1966065229381 for qualifier 253.0 of compound Benzo(b)fluoranthene; previous value = 157.268065765652			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:56 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:56 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:56 AM	Set PeakFilterThresholdValue = 386.411249999997 for compound Benzo(k)fluoranthene; previous value = 1003.41328761145			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:57 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:57 AM	No parameter change for PeakFilterThreshold			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:57 AM	Set PeakFilterThresholdValue = 88.9221430187413 for qualifier 253.0 of compound Benzo(k)fluoranthene; previous value = 231.172355781881			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:57 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:57 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:58 AM	Set PeakFilterThresholdValue = 285.618250000009 for compound Benzo(a)pyrene; previous value = 623.737750000004			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:58 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:58 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:58 AM	Set PeakFilterThresholdValue = 67.2428298292366 for qualifier 253.0 of compound Benzo(a)pyrene; previous value = 147.866406529718			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:58 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:58 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:59 AM	Set PeakFilterThresholdValue = 266.112953496991 for compound Indeno(1,2,3-cd)pyrene; previous value = 513.001406921189			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:54:59 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:59 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:59 AM	Set PeakFilterThresholdValue = 76.9869880142317 for qualifier 138.0 of compound Indeno(1,2,3-cd)pyrene; previous value = 129.069984146015			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:54:59 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:55:00 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:55:00 AM	Set PeakFilterThresholdValue = 325.884361205036 for compound Dibenzo(a,h)anthracene; previous value = 575.583630389075			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:55:00 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:55:00 AM	No parameter change for PeakFilterThreshold			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:55:00 AM	Set PeakFilterThresholdValue = 81.8984960160734 for qualifier 279.0 of compound Dibenzo(a,h)anthracene; previous value = 148.80303070392			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:55:00 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:55:01 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:55:01 AM	Set PeakFilterThresholdValue = 78.5354573917998 for qualifier 139.0 of compound Dibenzo(a,h)anthracene; previous value = 105.230153069532			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:55:01 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:55:01 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:55:01 AM	Set PeakFilterThresholdValue = 403.29425 for compound Benzo(g,h,i)perylene; previous value = 850.864177295763			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:55:02 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:55:02 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:55:02 AM	Set PeakFilterThresholdValue = 113.117519663444 for qualifier 138.0 of compound Benzo(g,h,i)perylene; previous value = 169.839410707477			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:55:02 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:55:02 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:55:03 AM	Set PeakFilterThresholdValue = 93.7669618316075 for qualifier 277.0 of compound Benzo(g,h,i)perylene; previous value = 208.343339694147			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:55:03 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:55:03 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:55:03 AM	Set PeakFilterThresholdValue = 142.440000000001 for compound Nitrobenzene-d5; previous value = 257.376672942736			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:55:03 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:55:04 AM	No parameter change for PeakFilterThreshold			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:55:04 AM	Set PeakFilterThresholdValue = 52.7133211898051 for qualifier 54.0 of compound Nitrobenzene-d5; previous value = 79.5320739966782			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:55:04 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:55:04 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:55:04 AM	Set PeakFilterThresholdValue = 52.1520225575144 for qualifier 128.0 of compound Nitrobenzene-d5; previous value = 78.2812723412894			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:55:04 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:55:05 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:55:05 AM	Set PeakFilterThresholdValue = 430.332750000005 for compound 2-Fluorobiphenyl; previous value = 927.30465			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:55:05 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:55:05 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:55:05 AM	Set PeakFilterThresholdValue = 163.741114532514 for qualifier 171.0 of compound 2-Fluorobiphenyl; previous value = 349.376072801849			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:55:05 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:55:06 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:55:06 AM	Set PeakFilterThresholdValue = 292.131788617147 for compound Terphenyl-d14; previous value = 520.464385855652			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:55:06 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:55:06 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:55:06 AM	Set PeakFilterThresholdValue = 56.0901280720104 for qualifier 122.0 of compound Terphenyl-d14; previous value = 71.4811505716088			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:55:06 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:55:07 AM	No parameter change for PeakFilterThreshold			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:55:07 AM	Set PeakFilterThresholdValue = 307.533749999996 for compound o-Terphenyl; previous value = 708.889818118197			✓	
CmdSetMethodTargetCompoundAttribute	BL2000\jheine	1/17/2022 8:55:07 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:55:07 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:55:07 AM	Set PeakFilterThresholdValue = 215.963649692389 for qualifier 229.0 of compound o-Terphenyl; previous value = 473.375347897728			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:55:07 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:55:07 AM	No parameter change for PeakFilterThreshold			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:55:08 AM	Set PeakFilterThresholdValue = 143.562068278791 for qualifier 215.0 of compound o-Terphenyl; previous value = 306.221532169349			✓	
CmdSetMethodTargetQualifierAttribute	BL2000\jheine	1/17/2022 8:55:08 AM	No parameter change for ThresholdNumberOfPeaks			✓	
CmdApplyMethodToAllSamples	BL2000\jheine	1/17/2022 8:55:15 AM	Apply method to all samples			✓	
CmdMethodClear	BL2000\jheine	1/17/2022 8:55:15 AM	Clear method			✓	
CmdEndMethodEditing	BL2000\jheine	1/17/2022 8:55:16 AM	End method editing			✓	
CmdQuantitate	BL2000\jheine	1/17/2022 8:55:23 AM	Quantitate all compounds in all samples			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 8:55:33 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1419.D			✓	
CmdSaveBatchTable	BL2000\jheine	1/17/2022 8:55:36 AM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\QuantResults\011422 bna SIM 2.batch.bin			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdImportSamplesFromWorklist	BL2000\jheine	1/17/2022 8:56:15 AM	Add samples from worklist: \\MASSHUNTER\Org\Data\SV5975.I\sh 011422\2 e8270c bna SIM\Jan1429.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011422\2 e8270c bna SIM\Jan1428.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011422\2 e8270c bna SIM\Jan1427.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011422\2 e8270c bna SIM\Jan1426.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011422\2 e8270c bna SIM\Jan1425.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011422\2 e8270c bna SIM\Jan1424.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011422\2 e8270c bna SIM\Jan1423.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011422\2 e8270c bna SIM\Jan1422.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011422\2 e8270c bna SIM\Jan1421.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011422\2 e8270c bna SIM\Jan1420.D			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 8:56:23 AM	Set SampleType = Blank for sample Jan1420.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 8:56:26 AM	Set SampleType = Blank for sample Jan1421.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 8:56:30 AM	Set SampleType = Matrix for sample Jan1422.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 8:56:34 AM	Set SampleType = Matrix for sample Jan1424.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 8:56:38 AM	Set SampleType = MatrixDup for sample Jan1425.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 8:56:43 AM	Set MatrixSpikeGroup = B21120800- 003D for sample Jan1423.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 8:56:44 AM	Set MatrixSpikeGroup = B21120800- 003D for sample Jan1424.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 8:56:45 AM	Set MatrixSpikeGroup = B21120800- 003D for sample Jan1425.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 8:56:50 AM	Set MatrixSpikeGroup = MB-162910- 162494-162167 for sample Jan1420.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 8:56:51 AM	Set MatrixSpikeGroup = MB-162910- 162494-162167 for sample Jan1422.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 8:56:55 AM	Set SampleInformation = MatrixA for sample Jan1422.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 8:57:01 AM	Set SampleInformation = MatrixA for sample Jan1424.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 8:57:03 AM	Set SampleInformation = MatrixA for sample Jan1425.D; previous value =			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdQuantitate	BL2000\jheine	1/17/2022 8:57:11 AM	Quantitate all compounds in all samples			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 8:57:32 AM	Manually integrate compound Acenaphthene in sample Jan1420.D, from x, y = 8.025, 87 to 8.150, 69, result = 136; previous integration is from x, y = 7.971, 70 to 8.150, 69 and previous response = 1499.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:57:34 AM	Drop baseline for compound Acenaphthene in sample Jan1420.D to y = 69, new integration is from x, y = 8.025, 69 to 8.150, 69 and new response = 206; previous integration is from x, y = 8.025, 87 to 8.150, 69 and previous response = 136.			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 8:57:37 AM	Zero out primary peak of compound Acenaphthene in sample Jan1420.D			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	1/17/2022 8:57:45 AM	Split peak for compound Anthracene in sample Jan1420.D and keep right peak, new integration is from x, y = 9.842, 71.7835599296537 to 9.891, 71.7835599296537 and new response = 251, previous integration is from x, y = 9.743, 72 to 9.891, 72 and previous response = 2026.			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 8:57:47 AM	Zero out primary peak of compound Anthracene in sample Jan1420.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 8:57:54 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1420.D			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	1/17/2022 8:57:59 AM	Split peak for compound Phenanthrene in sample Jan1420.D and keep left peak, new integration is from x, y = 9.743, 71.7835599296537 to 9.842, 71.7835599296537 and new response = 1775, previous integration is from x, y = 9.743, 72 to 9.891, 72 and previous response = 2026.			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	1/17/2022 8:58:04 AM	Split qualifier 176.0 of compound Phenanthrene in sample Jan1420.D and keep left peak, new integration is from x, y = 9.756, 62.3074283578283 to 9.830, 62.9612862917004 and new response = 313, previous integration is from x, y = 9.756, 62 to 9.891, 64 and previous response = 363.			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 8:58:09 AM	Zero out primary peak of compound Chrysene in sample Jan1420.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 8:58:13 AM	Zero out primary peak of compound Naphthalene in sample Jan1420.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 8:58:17 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1420.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 8:58:41 AM	Manually integrate compound o-Terphenyl in sample Jan1421.D from x, y = 10.262, 56 to 10.386, 66; result = 70			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/17/2022 8:58:42 AM	Snap baseline for compound o-Terphenyl in sample Jan1421.D, from x = 10.262 to x = 10.386, new integration is from x, y = 10.262, 53 to 10.386, 53 and new response = 131; previous integration is from x, y = 10.262, 56 to 10.386, 66 and previous response = 70.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:58:43 AM	Drop baseline for compound o-Terphenyl in sample Jan1421.D to y = 53, new integration is from x, y = 10.262, 53 to 10.386, 53 and new response = 131; previous integration is from x, y = 10.262, 53 to 10.386, 53 and previous response = 131.			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 8:58:46 AM	Zero out primary peak of compound o-Terphenyl in sample Jan1421.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 8:59:08 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1421.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 8:59:16 AM	Manually integrate compound Acenaphthene in sample Jan1421.D, from x, y = 8.026, 92 to 8.150, 61, result = 118; previous integration is from x, y = 7.977, 61 to 8.150, 61 and previous response = 1352.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:59:19 AM	Drop baseline for compound Acenaphthene in sample Jan1421.D to y = 61, new integration is from x, y = 8.026, 61 to 8.150, 61 and new response = 234; previous integration is from x, y = 8.026, 92 to 8.150, 61 and previous response = 118.			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 8:59:22 AM	Zero out primary peak of compound Acenaphthene in sample Jan1421.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 8:59:26 AM	Zero out primary peak of compound Chrysene in sample Jan1421.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 8:59:29 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1421.D			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/17/2022 8:59:41 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1422.D, from x, y = 5.941, 702 to 6.041, 71, result = 4143; previous integration is from x, y = 5.904, 71 to 6.041, 71 and previous response = 9129.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:59:42 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1422.D to y = 71, new integration is from x, y = 5.941, 71 to 6.041, 71 and new response = 6037; previous integration is from x, y = 5.941, 702 to 6.041, 71 and previous response = 4143.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/17/2022 8:59:56 AM	Manually integrate qualifier 142.0 of compound 1-Methylnaphthalene in sample Jan1422.D from x, y = 6.877, 1298 to 7.015, 2073; result = 6842			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/17/2022 8:59:58 AM	Snap baseline for qualifier 142.0 of compound 1-Methylnaphthalene in sample Jan1422.D from x = 6.877 to x = 7.015, new integration is from x, y = 6.877, 406 to 7.015, 249 and new response = 18035; previous integration is from x, y = 6.877, 1298 to 7.015, 2073 and previous response = 6842.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 8:59:58 AM	Drop baseline for qualifier 142.0 of compound 1-Methylnaphthalene in sample Jan1422.D to y = 249, new integration is from x, y = 6.877, 249 to 7.015, 249 and new response = 18682; previous integration is from x, y = 6.877, 406 to 7.015, 249 and previous response = 18035.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 9:01:26 AM	Manually integrate compound Acenaphthene in sample Jan1423.D, from x, y = 8.025, 96 to 8.138, 62, result = 141; previous integration is from x, y = 7.976, 62 to 8.138, 62 and previous response = 1373.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 9:01:28 AM	Drop baseline for compound Acenaphthene in sample Jan1423.D to y = 62, new integration is from x, y = 8.025, 62 to 8.138, 62 and new response = 256; previous integration is from x, y = 8.025, 96 to 8.138, 62 and previous response = 141.			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 9:01:32 AM	Zero out primary peak of compound Acenaphthene in sample Jan1423.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 9:01:35 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1423.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 9:01:37 AM	Zero out primary peak of compound Chrysene in sample Jan1423.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 9:01:38 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1423.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/17/2022 9:01:51 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1424.D, from x, y = 5.941, 590 to 6.041, 71, result = 5843; previous integration is from x, y = 5.902, 71 to 6.041, 71 and previous response = 10522.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 9:01:52 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1424.D to y = 71, new integration is from x, y = 5.941, 71 to 6.041, 71 and new response = 7398; previous integration is from x, y = 5.941, 590 to 6.041, 71 and previous response = 5843.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/17/2022 9:02:34 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1425.D, from x, y = 5.941, 790 to 6.041, 69, result = 4792; previous integration is from x, y = 5.904, 69 to 6.041, 69 and previous response = 9617.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 9:02:36 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1425.D to y = 69, new integration is from x, y = 5.941, 69 to 6.041, 69 and new response = 6954; previous integration is from x, y = 5.941, 790 to 6.041, 69 and previous response = 4792.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/17/2022 9:02:47 AM	Manually integrate qualifier 153.0 of compound Acenaphthylene in sample Jan1425.D from x, y = 7.814, 1962 to 7.876, 5369; result = -8074			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/17/2022 9:02:49 AM	Snap baseline for qualifier 153.0 of compound Acenaphthylene in sample Jan1425.D from x = 7.814 to x = 7.876, new integration is from x, y = 7.814, 98 to 7.876, 293 and new response = 4898; previous integration is from x, y = 7.814, 1962 to 7.876, 5369 and previous response = -8074.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 9:02:49 AM	Drop baseline for qualifier 153.0 of compound Acenaphthylene in sample Jan1425.D to y = 98, new integration is from x, y = 7.814, 98 to 7.876, 98 and new response = 5262; previous integration is from x, y = 7.814, 98 to 7.876, 293 and previous response = 4898.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/17/2022 9:03:47 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1426.D, from x, y = 5.941, 443 to 6.003, 115, result = 1756; previous integration is from x, y = 5.910, 115 to 6.003, 115 and previous response = 5674.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 9:03:49 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1426.D to y = 115, new integration is from x, y = 5.941, 115 to 6.003, 115 and new response = 2370; previous integration is from x, y = 5.941, 443 to 6.003, 115 and previous response = 1756.			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	1/17/2022 9:03:58 AM	Split peak for compound Anthracene in sample Jan1426.D and keep right peak, new integration is from x, y = 9.756, 90.634756141425 to 9.891, 93.0942121544834 and new response = 3509, previous integration is from x, y = 9.756, 91 to 9.891, 93 and previous response = 3509.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 9:04:04 AM	Manually integrate compound Anthracene in sample Jan1426.D, from x, y = 9.842, 521 to 9.891, 93, result = -236; previous integration is from x, y = 9.756, 91 to 9.891, 93 and previous response = 3509.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 9:04:05 AM	Drop baseline for compound Anthracene in sample Jan1426.D to y = 93, new integration is from x, y = 9.842, 93 to 9.891, 93 and new response = 399; previous integration is from x, y = 9.842, 521 to 9.891, 93 and previous response = -236.			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 9:04:08 AM	Zero out primary peak of compound Anthracene in sample Jan1426.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 9:04:13 AM	Manually integrate compound Fluorene in sample Jan1426.D, from x, y = 8.649, 78 to 8.723, 406, result = 1627; previous integration is from x, y = 8.649, 78 to 8.823, 78 and previous response = 2798.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 9:04:14 AM	Drop baseline for compound Fluorene in sample Jan1426.D to y = 78, new integration is from x, y = 8.649, 78 to 8.723, 78 and new response = 2362; previous integration is from x, y = 8.649, 78 to 8.723, 406 and previous response = 1627.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 9:04:30 AM	Manually integrate compound Acenaphthene in sample Jan1426.D, from x, y = 8.025, 386 to 8.088, 288, result = -311; previous integration is from x, y = 7.975, 82 to 8.150, 82 and previous response = 2170.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/17/2022 9:04:31 AM	Snap baseline for compound Acenaphthene in sample Jan1426.D, from x = 8.025 to x = 8.088, new integration is from x, y = 8.025, 160 to 8.088, 100 and new response = 462; previous integration is from x, y = 8.025, 386 to 8.088, 288 and previous response = -311.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 9:04:32 AM	Drop baseline for compound Acenaphthene in sample Jan1426.D to y = 100, new integration is from x, y = 8.025, 100 to 8.088, 100 and new response = 574; previous integration is from x, y = 8.025, 160 to 8.088, 100 and previous response = 462.			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 9:04:34 AM	Zero out primary peak of compound Acenaphthene in sample Jan1426.D			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	1/17/2022 9:04:38 AM	Split peak for compound Phenanthrene in sample Jan1426.D and keep left peak, new integration is from x, y = 9.756, 90.634756141425 to 9.891, 93.0942121544834 and new response = 3509, previous integration is from x, y = 9.756, 91 to 9.891, 93 and previous response = 3509.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 9:04:42 AM	Manually integrate compound Phenanthrene in sample Jan1426.D, from x, y = 9.756, 91 to 9.842, 541, result = 1984; previous integration is from x, y = 9.756, 91 to 9.891, 93 and previous response = 3509.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 9:04:43 AM	Drop baseline for compound Phenanthrene in sample Jan1426.D to y = 91, new integration is from x, y = 9.756, 91 to 9.842, 91 and new response = 3143; previous integration is from x, y = 9.756, 91 to 9.842, 541 and previous response = 1984.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 9:04:48 AM	Manually integrate compound Benzo(a)pyrene in sample Jan1426.D, from x, y = 18.363, 123 to 18.425, 194, result = -295; previous integration is from x, y = 18.463, 62 to 18.647, 63 and previous response = 1353.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/17/2022 9:04:49 AM	Snap baseline for compound Benzo(a)pyrene in sample Jan1426.D, from x = 18.363 to x = 18.425, new integration is from x, y = 18.363, 59 to 18.425, 60 and new response = 73; previous integration is from x, y = 18.363, 123 to 18.425, 194 and previous response = -295.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 9:04:50 AM	Drop baseline for compound Benzo(a)pyrene in sample Jan1426.D to y = 59, new integration is from x, y = 18.363, 59 to 18.425, 59 and new response = 75; previous integration is from x, y = 18.363, 59 to 18.425, 60 and previous response = 73.			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 9:04:53 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1426.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 9:05:00 AM	Manually integrate compound Chrysene in sample Jan1426.D, from x, y = 14.776, 167 to 14.863, 182, result = -375; previous integration is from x, y = 14.654, 54 to 14.776, 56 and previous response = 1469.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/17/2022 9:05:02 AM	Snap baseline for compound Chrysene in sample Jan1426.D, from x = 14.776 to x = 14.863, new integration is from x, y = 14.776, 120 to 14.863, 66 and new response = 50; previous integration is from x, y = 14.776, 167 to 14.863, 182 and previous response = -375.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 9:05:02 AM	Drop baseline for compound Chrysene in sample Jan1426.D to y = 66, new integration is from x, y = 14.776, 66 to 14.863, 66 and new response = 191; previous integration is from x, y = 14.776, 120 to 14.863, 66 and previous response = 50.			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 9:05:04 AM	Zero out primary peak of compound Chrysene in sample Jan1426.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 9:05:12 AM	Manually integrate compound Acenaphthylene in sample Jan1426.D, from x, y = 7.813, 106 to 7.838, 119, result = 154; previous integration is from x, y = 8.025, 112 to 8.088, 113 and previous response = 868.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 9:05:13 AM	Drop baseline for compound Acenaphthylene in sample Jan1426.D to y = 106, new integration is from x, y = 7.813, 106 to 7.838, 106 and new response = 163; previous integration is from x, y = 7.813, 106 to 7.838, 119 and previous response = 154.			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 9:05:14 AM	Zero out primary peak of compound Acenaphthylene in sample Jan1426.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdZeroOutPeak	BL2000\jheine	1/17/2022 9:05:17 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1426.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 9:05:42 AM	Manually integrate compound Benzo(a)pyrene in sample Jan1427.D, from x, y = 18.363, 106 to 18.438, 174, result = -277; previous integration is from x, y = 18.463, 61 to 18.598, 63 and previous response = 1615.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/17/2022 9:05:44 AM	Snap baseline for compound Benzo(a)pyrene in sample Jan1427.D, from x = 18.363 to x = 18.438, new integration is from x, y = 18.363, 57 to 18.438, 58 and new response = 90; previous integration is from x, y = 18.363, 106 to 18.438, 174 and previous response = -277.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 9:05:45 AM	Drop baseline for compound Benzo(a)pyrene in sample Jan1427.D to y = 57, new integration is from x, y = 18.363, 57 to 18.438, 57 and new response = 92; previous integration is from x, y = 18.363, 57 to 18.438, 58 and previous response = 90.			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 9:05:47 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1427.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 9:05:51 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1427.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 9:05:56 AM	Manually integrate compound Chrysene in sample Jan1427.D, from x, y = 14.776, 157 to 14.876, 162, result = -362; previous integration is from x, y = 14.665, 53 to 14.776, 53 and previous response = 1662.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/17/2022 9:05:58 AM	Snap baseline for compound Chrysene in sample Jan1427.D, from x = 14.776 to x = 14.876, new integration is from x, y = 14.776, 123 to 14.876, 64 and new response = 34; previous integration is from x, y = 14.776, 157 to 14.876, 162 and previous response = -362.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 9:05:58 AM	Drop baseline for compound Chrysene in sample Jan1427.D to y = 64, new integration is from x, y = 14.776, 64 to 14.876, 64 and new response = 210; previous integration is from x, y = 14.776, 123 to 14.876, 64 and previous response = 34.			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 9:06:00 AM	Zero out primary peak of compound Chrysene in sample Jan1427.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 9:06:11 AM	Manually integrate compound Anthracene in sample Jan1427.D, from x, y = 9.842, 116 to 9.941, 113, result = -38; previous integration is from x, y = 9.732, 66 to 9.842, 66 and previous response = 680.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/17/2022 9:06:12 AM	Snap baseline for compound Anthracene in sample Jan1427.D, from x = 9.842 to x = 9.941, new integration is from x, y = 9.842, 91 to 9.941, 72 and new response = 156; previous integration is from x, y = 9.842, 116 to 9.941, 113 and previous response = -38.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 9:06:13 AM	Drop baseline for compound Anthracene in sample Jan1427.D to y = 72, new integration is from x, y = 9.842, 72 to 9.941, 72 and new response = 212; previous integration is from x, y = 9.842, 91 to 9.941, 72 and previous response = 156.			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 9:06:14 AM	Zero out primary peak of compound Anthracene in sample Jan1427.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 9:06:20 AM	Manually integrate compound Acenaphthene in sample Jan1427.D, from x, y = 8.026, 91 to 8.138, 64, result = 181; previous integration is from x, y = 7.977, 64 to 8.138, 64 and previous response = 1482.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 9:06:21 AM	Drop baseline for compound Acenaphthene in sample Jan1427.D to y = 64, new integration is from x, y = 8.026, 64 to 8.138, 64 and new response = 270; previous integration is from x, y = 8.026, 91 to 8.138, 64 and previous response = 181.			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 9:06:22 AM	Zero out primary peak of compound Acenaphthene in sample Jan1427.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 9:06:32 AM	Zero out primary peak of compound 1-Methylnaphthalene in sample Jan1427.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 9:06:34 AM	Zero out primary peak of compound 2-Methylnaphthalene in sample Jan1427.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 9:06:36 AM	Zero out primary peak of compound Naphthalene in sample Jan1427.D			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/17/2022 9:06:54 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1428.D, from x, y = 5.941, 2562 to 6.003, 2593, result = -5204; previous integration is from x, y = 5.914, 186 to 6.046, 186 and previous response = 8128.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateS napBaseline	BL2000\jheine	1/17/2022 9:06:56 AM	Snap baseline for qualifier 102.0 of compound Naphthalene in sample Jan1428.D from x = 5.941 to x = 6.003, new integration is from x, y = 5.941, 1648 to 6.003, 284 and new response = 833; previous integration is from x, y = 5.941, 2562 to 6.003, 2593 and previous response = -5204.			✓	
CmdManuallyIntegrate DropBaseline	BL2000\jheine	1/17/2022 9:06:57 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1428.D to y = 284, new integration is from x, y = 5.941, 284 to 6.003, 284 and new response = 3387; previous integration is from x, y = 5.941, 1648 to 6.003, 284 and previous response = 833.			✓	
CmdManuallyIntegrate QualifierPeak	BL2000\jheine	1/17/2022 9:07:02 AM	Manually integrate qualifier 129.0 of compound Naphthalene in sample Jan1428.D, from x, y = 5.941, 398 to 6.003, 338, result = 3606; previous integration is from x, y = 5.920, 338 to 6.003, 338 and previous response = 3908.			✓	
CmdManuallyIntegrate DropBaseline	BL2000\jheine	1/17/2022 9:07:03 AM	Drop baseline for qualifier 129.0 of compound Naphthalene in sample Jan1428.D to y = 338, new integration is from x, y = 5.941, 338 to 6.003, 338 and new response = 3718; previous integration is from x, y = 5.941, 398 to 6.003, 338 and previous response = 3606.			✓	
CmdManuallyIntegrate QualifierPeak	BL2000\jheine	1/17/2022 9:07:16 AM	Manually integrate qualifier 167.0 of compound Fluorene in sample Jan1428.D, from x, y = 8.650, 195 to 8.674, 326, result = 320; previous integration is from x, y = 8.650, 195 to 8.711, 204 and previous response = 1013.			✓	
CmdManuallyIntegrate DropBaseline	BL2000\jheine	1/17/2022 9:07:17 AM	Drop baseline for qualifier 167.0 of compound Fluorene in sample Jan1428.D to y = 195, new integration is from x, y = 8.650, 195 to 8.674, 195 and new response = 412; previous integration is from x, y = 8.650, 195 to 8.674, 326 and previous response = 320.			✓	
CmdManuallyIntegrateP eak	BL2000\jheine	1/17/2022 9:07:26 AM	Manually integrate compound Acenaphthene in sample Jan1428.D, from x, y = 8.026, 861 to 8.088, 632, result = -938; previous integration is from x, y = 7.982, 136 to 8.113, 136 and previous response = 3026.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/17/2022 9:07:28 AM	Snap baseline for compound Acenaphthene in sample Jan1428.D, from x = 8.026 to x = 8.088, new integration is from x, y = 8.026, 178 to 8.088, 153 and new response = 1234; previous integration is from x, y = 8.026, 861 to 8.088, 632 and previous response = -938.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 9:07:29 AM	Drop baseline for compound Acenaphthene in sample Jan1428.D to y = 153, new integration is from x, y = 8.026, 153 to 8.088, 153 and new response = 1280; previous integration is from x, y = 8.026, 178 to 8.088, 153 and previous response = 1234.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/17/2022 9:07:34 AM	Manually integrate qualifier 152.0 of compound Acenaphthene in sample Jan1428.D, from x, y = 8.026, 214 to 8.088, 236, result = 1804; previous integration is from x, y = 8.029, 588 to 8.056, 588 and previous response = 465.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 9:07:36 AM	Drop baseline for qualifier 152.0 of compound Acenaphthene in sample Jan1428.D to y = 214, new integration is from x, y = 8.026, 214 to 8.088, 214 and new response = 1844; previous integration is from x, y = 8.026, 214 to 8.088, 236 and previous response = 1804.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 9:07:43 AM	Manually integrate compound Anthracene in sample Jan1428.D, from x, y = 9.842, 349 to 9.892, 563, result = -536; previous integration is from x, y = 9.760, 142 to 9.842, 142 and previous response = 3298.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/17/2022 9:07:45 AM	Snap baseline for compound Anthracene in sample Jan1428.D, from x = 9.842 to x = 9.892, new integration is from x, y = 9.842, 177 to 9.892, 178 and new response = 290; previous integration is from x, y = 9.842, 349 to 9.892, 563 and previous response = -536.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 9:07:45 AM	Drop baseline for compound Anthracene in sample Jan1428.D to y = 177, new integration is from x, y = 9.842, 177 to 9.892, 177 and new response = 292; previous integration is from x, y = 9.842, 177 to 9.892, 178 and previous response = 290.			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 9:07:49 AM	Zero out primary peak of compound Anthracene in sample Jan1428.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateSplit	BL2000\jheine	1/17/2022 9:07:53 AM	Split qualifier 176.0 of compound Phenanthrene in sample Jan1428.D and keep left peak, new integration is from x, y = 9.780, 80.3551302990649 to 9.892, 79.5341563220301 and new response = 623, previous integration is from x, y = 9.780, 80 to 9.892, 80 and previous response = 623.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/17/2022 9:07:57 AM	Manually integrate qualifier 176.0 of compound Phenanthrene in sample Jan1428.D, from x, y = 9.780, 80 to 9.842, 148, result = 502; previous integration is from x, y = 9.780, 80 to 9.892, 80 and previous response = 623.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 9:07:58 AM	Drop baseline for qualifier 176.0 of compound Phenanthrene in sample Jan1428.D to y = 80, new integration is from x, y = 9.780, 80 to 9.842, 80 and new response = 627; previous integration is from x, y = 9.780, 80 to 9.842, 148 and previous response = 502.			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 9:08:02 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1428.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 9:08:11 AM	Manually integrate compound Chrysene in sample Jan1428.D, from x, y = 14.776, 78 to 14.888, 53, result = 113; previous integration is from x, y = 14.664, 53 to 14.888, 53 and previous response = 1608.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 9:08:12 AM	Drop baseline for compound Chrysene in sample Jan1428.D to y = 53, new integration is from x, y = 14.776, 53 to 14.888, 53 and new response = 199; previous integration is from x, y = 14.776, 78 to 14.888, 53 and previous response = 113.			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 9:08:14 AM	Zero out primary peak of compound Chrysene in sample Jan1428.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 9:08:22 AM	Manually integrate compound Acenaphthylene in sample Jan1428.D, from x, y = 7.814, 149 to 7.839, 209, result = 367; previous integration is from x, y = 7.739, 300 to 7.789, 202 and previous response = 1266.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 9:08:24 AM	Drop baseline for compound Acenaphthylene in sample Jan1428.D to y = 149, new integration is from x, y = 7.814, 149 to 7.839, 149 and new response = 412; previous integration is from x, y = 7.814, 149 to 7.839, 209 and previous response = 367.			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 9:08:25 AM	Zero out primary peak of compound Acenaphthylene in sample Jan1428.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdZeroOutPeak	BL2000\jheine	1/17/2022 9:08:27 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1428.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 9:08:44 AM	Manually integrate compound 2-Methylnaphthalene in sample Jan1429.D, from x, y = 6.777, 139 to 6.827, 190, result = 51; previous integration is from x, y = 6.865, 88 to 6.965, 89 and previous response = 1313.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/17/2022 9:08:45 AM	Snap baseline for compound 2-Methylnaphthalene in sample Jan1429.D, from x = 6.777 to x = 6.827, new integration is from x, y = 6.777, 94 to 6.827, 101 and new response = 251; previous integration is from x, y = 6.777, 139 to 6.827, 190 and previous response = 51.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 9:08:46 AM	Drop baseline for compound 2-Methylnaphthalene in sample Jan1429.D to y = 94, new integration is from x, y = 6.777, 94 to 6.827, 94 and new response = 262; previous integration is from x, y = 6.777, 94 to 6.827, 101 and previous response = 251.			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 9:08:50 AM	Zero out primary peak of compound 2-Methylnaphthalene in sample Jan1429.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 9:09:01 AM	Manually integrate compound Acenaphthene in sample Jan1429.D, from x, y = 8.025, 250 to 8.100, 243, result = -536; previous integration is from x, y = 7.966, 66 to 8.150, 66 and previous response = 1457.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/17/2022 9:09:01 AM	Snap baseline for compound Acenaphthene in sample Jan1429.D, from x = 8.025 to x = 8.100, new integration is from x, y = 8.025, 155 to 8.100, 81 and new response = 40; previous integration is from x, y = 8.025, 250 to 8.100, 243 and previous response = -536.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 9:09:01 AM	Drop baseline for compound Acenaphthene in sample Jan1429.D to y = 81, new integration is from x, y = 8.025, 81 to 8.100, 81 and new response = 206; previous integration is from x, y = 8.025, 155 to 8.100, 81 and previous response = 40.			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 9:09:03 AM	Zero out primary peak of compound Acenaphthene in sample Jan1429.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/17/2022 9:09:23 AM	Manually integrate qualifier 115.0 of compound 1-Methylnaphthalene in sample Jan1429.D, from x, y = 6.877, 206 to 6.927, 226, result = 704; previous integration is from x, y = 6.877, 206 to 7.002, 203 and previous response = 987.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 9:09:41 AM	Drop baseline for qualifier 115.0 of compound 1-Methylnaphthalene in sample Jan1429.D to y = 206, new integration is from x, y = 6.877, 206 to 6.927, 206 and new response = 733; previous integration is from x, y = 6.877, 206 to 6.927, 226 and previous response = 704.			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 9:10:10 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1429.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/17/2022 9:10:15 AM	Manually integrate compound Chrysene in sample Jan1429.D, from x, y = 14.776, 153 to 14.876, 121, result = -257; previous integration is from x, y = 14.664, 52 to 14.776, 52 and previous response = 1611.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/17/2022 9:10:17 AM	Snap baseline for compound Chrysene in sample Jan1429.D, from x = 14.776 to x = 14.876, new integration is from x, y = 14.776, 114 to 14.876, 62 and new response = 35; previous integration is from x, y = 14.776, 153 to 14.876, 121 and previous response = -257.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/17/2022 9:10:17 AM	Drop baseline for compound Chrysene in sample Jan1429.D to y = 62, new integration is from x, y = 14.776, 62 to 14.876, 62 and new response = 190; previous integration is from x, y = 14.776, 114 to 14.876, 62 and previous response = 35.			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 9:10:19 AM	Zero out primary peak of compound Chrysene in sample Jan1429.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 9:10:21 AM	Zero out primary peak of compound Naphthalene in sample Jan1429.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 9:10:24 AM	Zero out primary peak of compound Anthracene in sample Jan1429.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/17/2022 9:10:25 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1429.D			✓	
CmdSaveBatchTable	BL2000\jheine	1/17/2022 9:10:30 AM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\QuantResults\011422 bna SIM2.batch.bin			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSaveBatchTable	BL2000\jheine	1/17/2022 9:10:38 AM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011422\2 e8270c bna SIM\QuantResults\011422 bna SIM 2.batch.bin			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 9:11:16 AM	Set SampleApproved = True for sample Jan1410.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 9:11:19 AM	Set SampleApproved = True for sample Jan1411.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 9:11:21 AM	Set SampleApproved = True for sample Jan1412.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 9:11:22 AM	Set SampleApproved = True for sample Jan1413.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 9:11:23 AM	Set SampleApproved = True for sample Jan1414.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 9:11:23 AM	Set SampleApproved = True for sample Jan1415.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 9:11:24 AM	Set SampleApproved = True for sample Jan1416.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 9:11:26 AM	Set SampleApproved = True for sample Jan1417.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 9:11:29 AM	Set SampleApproved = True for sample Jan1418.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/17/2022 9:11:30 AM	Set SampleApproved = True for sample Jan1419.D; previous value = False			✓	
CmdSaveBatchTable	BL2000\jheine	1/17/2022 9:11:33 AM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011422\2 e8270c bna SIM\QuantResults\011422 bna SIM 2.batch.bin			✓	
CmdSaveBatchTable	BL2000\jheine	1/17/2022 9:13:13 AM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011422\2 e8270c bna SIM\QuantResults\011422 bna SIM 2.batch.bin			✓	
CmdSaveBatchTable	BL2000\jheine	1/17/2022 9:19:06 AM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011422\2 e8270c bna SIM\QuantResults\011422 bna SIM 2.batch.bin			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdOpenBatchTable	BL2000\jheine	2/4/2022 3:18:18 PM	Open batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011422\2 e8270c bna SIM\011422 bna SIM 2.batch.bin			✓	
CmdQuantitate	BL2000\jheine	2/4/2022 3:28:19 PM	Quantitate all compounds in all samples			✓	
CmdQuantitate	BL2000\jheine	2/4/2022 3:29:06 PM	Quantitate all compounds in all samples			✓	
CmdSaveBatchTable	BL2000\jheine	2/4/2022 3:29:09 PM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011422\2 e8270c bna SIM\QuantResults\011422 bna SIM 2.batch.bin			✓	
GenerateReport	BL2000\jheine	2/4/2022 3:30:44 PM	Generates report - Method: D:\Org\reports\GCMSSSEMI Report Templates\Calibration\Gen_Calibration. m, Output Path: \\MASSHUNTER\Org\Data\SV5975.I\sh 011422\2 e8270c bna SIM\QuantReports\			✓	
GenerateReport	BL2000\jheine	2/4/2022 3:43:20 PM	Generates report - Method: D:\Org\reports\GCMSSSEMI Report Templates\Calibration\lcspike_rpt.m, Output Path: \\MASSHUNTER\Org\Data\SV5975.I\sh 011422\2 e8270c bna SIM\QuantReports\			✓	
GenerateReport	BL2000\jheine	2/4/2022 3:44:47 PM	Generates report - Method: D:\Org\reports\GCMSSSEMI Report Templates\Calibration\init_cal_rpt.m, Output Path: \\MASSHUNTER\Org\Data\SV5975.I\sh 011422\2 e8270c bna SIM\QuantReports\			✓	
GenerateReport	BL2000\jheine	2/4/2022 3:46:16 PM	Generates report - Method: D:\Org\reports\GCMSSSEMI Report Templates\Calibration\Gen_ResultsSu mmmary.m, Output Path: \\MASSHUNTER\Org\Data\SV5975.I\sh 011422\2 e8270c bna SIM\QuantReports\			✓	
GenerateReport	BL2000\jheine	2/4/2022 3:51:36 PM	Generates report - Method: D:\Org\reports\GCMSSSEMI Report Templates\Calibration\Env_QuantResul ts_wGraphics+Chromatogram.m, Output Path: \\MASSHUNTER\Org\Data\SV5975.I\sh 011422\2 e8270c bna SIM\QuantReports\			✓	

Energy Laboratories Inc

ANALYTICAL RUN Summary

04-Feb-22

Run ID SV5975.I_220118A

Run Start Date: 1/18/2022
Analyst: John P. Heine
Ical:
Column ID: ZB-SemiVolatiles
Comments:

Std ID	Std Name	Std Amount	Std Units	Samp Amount	Samp Units	SampType	Expiration Date
dcmsvoc13	DCM						11/17/2022
sv100506	BNA low 50 ug/mL	8	ul	192	ul	CCV	3/31/2022
sv100703	BNA Internals 2000 ug/mL	2	ul	100	ul	SAMP	5/31/2022
sv100801	BNA 2nd source 200ug/mL	2	ul	198	ul	ICV	10/1/2022
sv83311	DFTPP 1000 ug/mL	50	ul	50	ul	TUNE	10/31/2022

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985900	Jan1801_D_TU	SVOC-8270-DF	TUNE	V5975.I\sh0118221	18/2022 3:31:0	1	R373371		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
127, % of mass 198	A	%	59.6	59.6		100	0	0	0	0.01	0	60%	40	60	0%	
197, % of mass 198	A	%	0	0		100	0	0	0	0.01	0	0%	0	0.99	0%	
198, Base Peak	A	%	100	100		100	0	0	0	0.01	0	100%	100	100	0%	
199, % of mass 198	A	%	7.2	7.2		100	0	0	0	0.01	0	7%	5	9	0%	
275, % of mass 198	A	%	26.7	26.7		100	0	0	0	0.01	0	27%	10	30	0%	
365, % of mass 198	A	%	3.2	3.2		100	0	0	0	0.01	0	3%	1	99.99	0%	
441, % of mass 443	A	%	89	89		100	0	0	0	0.01	0	89%	0.01	150	0%	
442, % of mass 198	A	%	66.6	66.6		100	0	0	0	0.01	0	67%	40	100	0%	
443, % of mass 442	A	%	19.2	19.2		100	0	0	0	0.01	0	19%	17	23	0%	
51, % of mass 198	A	%	46.9	46.9		100	0	0	0	0.01	0	47%	30	60	0%	
68, % of mass 69	A	%	0	0		100	0	0	0	0.01	0	0%	0	1.99	0%	
70, % of mass 69	A	%	0.6	0.6		100	0	0	0	0.01	0	1%	0	1.99	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985901	18-Jan-22_CCV	SVOC-8270C-SI	CCV	V5975.I\sh0118221/18/2022	3:55:2	1	R373371		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	1.84345	1.84345		2	0	0	0.0206	0.1	10	92%	80	120	0%	
2-Methylnaphthalene	A	ug/L	1.90491	1.90491		2	0	0	0.0176	0.1	10	95%	80	120	0%	
Acenaphthene	A	ug/L	1.70355	1.70355		2	0	0	0.0317	0.1	10	85%	80	120	0%	
Acenaphthylene	A	ug/L	1.79533	1.79533		2	0	0	0.025	0.1	10	90%	80	120	0%	
Anthracene	A	ug/L	2.01291	2.01291		2	0	0	0.0283	0.1	10	101%	80	120	0%	
Benzo(a)anthracene	A	ug/L	2.12247	2.12247		2	0	0	0.0272	0.1	10	106%	80	120	0%	
Benzo(a)pyrene	A	ug/L	2.11128	2.11128		2	0	0	0.0347	0.1	10	106%	80	120	0%	
Benzo(b)fluoranthene	A	ug/L	1.83166	1.83166		2	0	0	0.0226	0.1	10	92%	80	120	0%	
Benzo(g,h,i)perylene	A	ug/L	1.94935	1.94935		2	0	0	0.0267	0.1	10	97%	80	120	0%	
Benzo(k)fluoranthene	A	ug/L	1.9817	1.9817		2	0	0	0.0295	0.1	10	99%	80	120	0%	
Chrysene	A	ug/L	1.8366	1.8366		2	0	0	0.0458	0.1	10	92%	80	120	0%	
Dibenzo(a,h)anthracene	A	ug/L	1.82081	1.82081		2	0	0	0.0367	0.1	10	91%	80	120	0%	
Fluoranthene	A	ug/L	1.79769	1.79769		2	0	0	0.0233	0.1	10	90%	80	120	0%	
Fluorene	A	ug/L	1.84676	1.84676		2	0	0	0.0225	0.1	10	92%	80	120	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	2.00611	2.00611		2	0	0	0.0491	0.1	10	100%	80	120	0%	
Naphthalene	A	ug/L	1.66681	1.66681		2	0	0	0.029	0.1	10	83%	80	120	0%	
Phenanthrene	A	ug/L	1.9307	1.9307		2	0	0	0.0295	0.1	10	97%	80	120	0%	
Pyrene	A	ug/L	2.00545	2.00545		2	0	0	0.0239	0.1	10	100%	80	120	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	80	120	0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1	10	0%	80	120	0%	
2-Fluorobiphenyl	S	ug/L	1.94532	1.94532		2	0	0	0.0444	0.1	10	97%	80	120	0%	
Nitrobenzene-d5	S	ug/L	1.83403	1.83403		2	0	0	0.0523	0.1	10	92%	80	120	0%	
Terphenyl-d14	S	ug/L	2.05995	2.05995		2	0	0	0.0563	0.1	10	103%	80	120	0%	
o-Terphenyl	X	ug/L	1.82764	1.82764		2	0	0	0.0654	0	0	91%	80	120	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985902	18-Jan-22_ISTB	SVOC-8270C-SI	SAMP	V5975.I\sh0118221/18/2022	4:27:4	1	R373371		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985902	18-Jan-22_ISTB	SVOC-8270C-SI	SAMP	V5975.I\sh0118221/18/2022	4:27:4	1	R373371		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0206	0.1	10	0%	0	0	0%	
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0176	0.1	10	0%	0	0	0%	
Acenaphthene	A	ug/L	0	0		0	0	0	0.0317	0.1	10	0%	0	0	0%	
Acenaphthylene	A	ug/L	0	0		0	0	0	0.025	0.1	10	0%	0	0	0%	
Anthracene	A	ug/L	0	0		0	0	0	0.0283	0.1	10	0%	0	0	0%	
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.0272	0.1	10	0%	0	0	0%	
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.0347	0.1	10	0%	0	0	0%	
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.0226	0.1	10	0%	0	0	0%	
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.0267	0.1	10	0%	0	0	0%	
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.0295	0.1	10	0%	0	0	0%	
Chrysene	A	ug/L	0	0		0	0	0	0.0458	0.1	10	0%	0	0	0%	
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.0367	0.1	10	0%	0	0	0%	
Fluoranthene	A	ug/L	0	0		0	0	0	0.0233	0.1	10	0%	0	0	0%	
Fluorene	A	ug/L	0	0		0	0	0	0.0225	0.1	10	0%	0	0	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.0491	0.1	10	0%	0	0	0%	
Naphthalene	A	ug/L	0	0		0	0	0	0.029	0.1	10	0%	0	0	0%	
Phenanthrene	A	ug/L	0	0		0	0	0	0.0295	0.1	10	0%	0	0	0%	
Pyrene	A	ug/L	0	0		0	0	0	0.0239	0.1	10	0%	0	0	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1	10	0%	0	0	0%	E
2-Fluorobiphenyl	S	ug/L	0	0		5	0	0	0.0444	0.1	10	0%	25	94	0%	S
Nitrobenzene-d5	S	ug/L	0	0		5	0	0	0.0523	0.1	10	0%	19	102	0%	S
Terphenyl-d14	S	ug/L	0	0		5	0	0	0.0563	0.1	10	0%	39	106	0%	S
o-Terphenyl	X	ug/L	0	0		200	0	0	0.0654	0	0	0%	40	140	0%	S

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985903	B22010212-001	SVOC-8270C-SI	SAMP	V5975.I\sh0118221/18/2022	5:00:1	1	162701	1/5/2022 1:1	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985903	B22010212-001	SVOC-8270C-SI	SAMP	V5975.I\sh0118221/18/2022	5:00:1	1	162701	1/5/2022 1:1	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.020188	0.1	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.017248	0.1	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.031066	0.1	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.0245	0.1	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.027734	0.1	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.026656	0.1	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.034006	0.1	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.022148	0.1	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.026166	0.1	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.02891	0.1	10	0%	0	0	0%	U
Chrysene	A	ug/L	0	0		0	0	0	0.044884	0.1	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.035966	0.1	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0	0		0	0	0	0.022834	0.1	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.02205	0.1	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.048118	0.1	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.02842	0.1	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.02891	0.1	10	0%	0	0	0%	U
Pyrene	A	ug/L	0	0		0	0	0	0.023422	0.1	10	0%	0	0	0%	U
1,4-Dichlorobenzene-d4	I	ug/L	40	39.2		0	0	0	0.098	0.1		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	39.2		0	0	0	0.098	0.1		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	39.2		0	0	0	0.098	0.1		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	39.2		0	0	0	0.098	0.1		0%	0	0	0%	
Perylene-d12	I	ug/L	40	39.2		0	0	0	0.098	0.1		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	39.2		0	0	0	0.098	0.1	10	0%	0	0	0%	E

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985904	B22010211-001	SVOC-8270C-SI	SAMP	V5975.I\sh0118221/18/2022	5:32:3	100	162701	1/5/2022 1:1	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	5.938	629.428		0	0	0	2.1836	10.6	10	0%	0	0	0%	
2-Methylnaphthalene	A	ug/L	8.51102	902.16812		0	0	0	1.8656	10.6	10	0%	0	0	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985905	LLCS-162800	SVOC-8270C-SI	LCS-DOD	V5975.I\sh0118221	18/2022 6:05:1	20	162800	1/10/2022 8:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
2-Fluorobiphenyl	S	ug/L	3.72314	74.4628		100	0	0	0.888	2	10	74%	53	106	0%	
Nitrobenzene-d5	S	ug/L	3.92807	78.5614		100	0	0	1.046	2	10	79%	55	111	0%	
Terphenyl-d14	S	ug/L	6.05682	121.1364		100	0	0	1.126	2	10	121%	58	132	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985906	LLCSD-162800	SVOC-8270C-SI	LCS-DOD	V5975.I\sh0118221	18/2022 6:37:2	1	162800	1/10/2022 8:	0	1E+07						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
2-Fluorobiphenyl	S	ug/L	3.24675	3.24675		5	0	0	0.0444	0.1	10	65%	53	106	0%	
Nitrobenzene-d5	S	ug/L	4.39731	4.39731		5	0	0	0.0523	0.1	10	88%	55	111	0%	
Terphenyl-d14	S	ug/L	5.52495	5.52495		5	0	0	0.0563	0.1	10	110%	58	132	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985907	LLCS-162889	SVOC-8270C-SI	LCS-DOD	V5975.I\sh0118221	18/2022 7:09:4	1	162889	1/12/2022 2:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	2.94513	2.94513		5	0	0	0.0206	0.1	10	59%	41	115	0%	
2-Methylnaphthalene	A	ug/L	3.50989	3.50989		5	0	0	0.0176	0.1	10	70%	39	114	0%	
Acenaphthene	A	ug/L	3.34772	3.34772		5	0	0	0.0317	0.1	10	67%	48	114	0%	
Acenaphthylene	A	ug/L	3.23056	3.23056		5	0	0	0.025	0.1	10	65%	35	121	0%	
Anthracene	A	ug/L	4.65305	4.65305		5	0	0	0.0283	0.1	10	93%	53	119	0%	
Benzo(a)anthracene	A	ug/L	5.02601	5.02601		5	0	0	0.0272	0.1	10	101%	59	120	0%	
Benzo(a)pyrene	A	ug/L	4.76667	4.76667		5	0	0	0.0347	0.1	10	95%	53	120	0%	
Benzo(b)fluoranthene	A	ug/L	4.90832	4.90832		5	0	0	0.0226	0.1	10	98%	53	126	0%	
Benzo(g,h,i)perylene	A	ug/L	4.67951	4.67951		5	0	0	0.0267	0.1	10	94%	44	128	0%	
Benzo(k)fluoranthene	A	ug/L	4.39214	4.39214		5	0	0	0.0295	0.1	10	88%	54	125	0%	
Chrysene	A	ug/L	4.69343	4.69343		5	0	0	0.0458	0.1	10	94%	57	120	0%	
Dibenzo(a,h)anthracene	A	ug/L	4.68976	4.68976		5	0	0	0.0367	0.1	10	94%	44	141	0%	
Fluoranthene	A	ug/L	4.47876	4.47876		5	0	0	0.0233	0.1	10	90%	58	120	0%	
Fluorene	A	ug/L	3.87627	3.87627		5	0	0	0.0225	0.1	10	78%	50	118	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	4.51092	4.51092		5	0	0	0.0491	0.1	10	90%	48	130	0%	
Naphthalene	A	ug/L	2.92266	2.92266		5	0	0	0.029	0.1	10	58%	43	114	0%	
Phenanthrene	A	ug/L	4.59141	4.59141		5	0	0	0.0295	0.1	10	92%	53	115	0%	
Pyrene	A	ug/L	4.46554	4.46554		5	0	0	0.0239	0.1	10	89%	53	121	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985907	LLCS-162889	SVOC-8270C-SI	LCS-DOD	V5975.I\sh0118221/18/2022	7:09:4	1	162889	1/12/2022 2:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1	10	0%			0%	
2-Fluorobiphenyl	S	ug/L	3.39211	3.39211		5	0	0	0.0444	0.1	10	68%	53	106	0%	
Nitrobenzene-d5	S	ug/L	4.06312	4.06312		5	0	0	0.0523	0.1	10	81%	55	111	0%	
Terphenyl-d14	S	ug/L	5.05279	5.05279		5	0	0	0.0563	0.1	10	101%	58	132	0%	
o-Terphenyl	X	ug/L	4.17682	4.17682		5	0	0	0.0654	0	0	84%	40	140	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985908	LLCSD-162889	SVOC-8270C-SI	LCSD-DOD	V5975.I\sh0118221/18/2022	7:42:0	1	162889	1/12/2022 2:	0	1E+07						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	2.36722	2.36722		5	0	2.94513	0.0206	0.1	10	47%	41	115	22%	
2-Methylnaphthalene	A	ug/L	2.72774	2.72774		5	0	3.50989	0.0176	0.1	10	55%	39	114	25%	
Acenaphthene	A	ug/L	2.79938	2.79938		5	0	3.34772	0.0317	0.1	10	56%	48	114	18%	
Acenaphthylene	A	ug/L	2.81421	2.81421		5	0	3.23056	0.025	0.1	10	56%	35	121	14%	
Anthracene	A	ug/L	4.53284	4.53284		5	0	4.65305	0.0283	0.1	10	91%	53	119	3%	
Benzo(a)anthracene	A	ug/L	5.13253	5.13253		5	0	5.02601	0.0272	0.1	10	103%	59	120	2%	
Benzo(a)pyrene	A	ug/L	4.92369	4.92369		5	0	4.76667	0.0347	0.1	10	98%	53	120	3%	
Benzo(b)fluoranthene	A	ug/L	5.11649	5.11649		5	0	4.90832	0.0226	0.1	10	102%	53	126	4%	
Benzo(g,h,i)perylene	A	ug/L	4.77174	4.77174		5	0	4.67951	0.0267	0.1	10	95%	44	128	2%	
Benzo(k)fluoranthene	A	ug/L	4.73216	4.73216		5	0	4.39214	0.0295	0.1	10	95%	54	125	7%	
Chrysene	A	ug/L	4.77576	4.77576		5	0	4.69343	0.0458	0.1	10	96%	57	120	2%	
Dibenzo(a,h)anthracene	A	ug/L	4.99191	4.99191		5	0	4.68976	0.0367	0.1	10	100%	44	141	6%	
Fluoranthene	A	ug/L	4.41864	4.41864		5	0	4.47876	0.0233	0.1	10	88%	58	120	1%	
Fluorene	A	ug/L	3.46982	3.46982		5	0	3.87627	0.0225	0.1	10	69%	50	118	11%	
Indeno(1,2,3-cd)pyrene	A	ug/L	4.82049	4.82049		5	0	4.51092	0.0491	0.1	10	96%	48	130	7%	
Naphthalene	A	ug/L	2.41921	2.41921		5	0	2.92266	0.029	0.1	10	48%	43	114	19%	
Phenanthrene	A	ug/L	4.3439	4.3439		5	0	4.59141	0.0295	0.1	10	87%	53	115	6%	
Pyrene	A	ug/L	4.53956	4.53956		5	0	4.46554	0.0239	0.1	10	91%	53	121	2%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985908	LLCSD-162889	SVOC-8270C-SI	LCSD-DOD	V5975.I\sh0118221/18/2022	7:42:0	1	162889	1/12/2022 2:	0	1E+07						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%				0%
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%				0%
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%				0%
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1	10	0%				0%
2-Fluorobiphenyl	S	ug/L	3.06148	3.06148		5	0	0	0.0444	0.1	10	61%	53	106		0%
Nitrobenzene-d5	S	ug/L	3.87605	3.87605		5	0	0	0.0523	0.1	10	78%	55	111		0%
Terphenyl-d14	S	ug/L	5.07681	5.07681		5	0	0	0.0563	0.1	10	102%	58	132		0%
o-Terphenyl	X	ug/L	4.01636	4.01636		5	0	4.17682	0.0654	0	0	80%	40	140		4%

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985909	MB-162889	SVOC-8270C-SI	MBLK	V5975.I\sh0118221/18/2022	8:14:2	1	162889	1/12/2022 2:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0206	0.1	10	0%				0%
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0176	0.1	10	0%				0%
Acenaphthene	A	ug/L	0	0		0	0	0	0.0317	0.1	10	0%				0%
Acenaphthylene	A	ug/L	0	0		0	0	0	0.025	0.1	10	0%				0%
Anthracene	A	ug/L	0	0		0	0	0	0.0283	0.1	10	0%				0%
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.0272	0.1	10	0%				0%
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.0347	0.1	10	0%				0%
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.0226	0.1	10	0%				0%
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.0267	0.1	10	0%				0%
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.0295	0.1	10	0%				0%
Chrysene	A	ug/L	0	0		0	0	0	0.0458	0.1	10	0%				0%
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.0367	0.1	10	0%				0%
Fluoranthene	A	ug/L	0	0		0	0	0	0.0233	0.1	10	0%				0%
Fluorene	A	ug/L	0	0		0	0	0	0.0225	0.1	10	0%				0%
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.0491	0.1	10	0%				0%
Naphthalene	A	ug/L	0	0		0	0	0	0.029	0.1	10	0%				0%
Phenanthrene	A	ug/L	0	0		0	0	0	0.0295	0.1	10	0%				0%
Pyrene	A	ug/L	0	0		0	0	0	0.0239	0.1	10	0%				0%
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%				0%
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%				0%
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%				0%
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%				0%

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985909	MB-162889	SVOC-8270C-SI	MBLK	V5975.I\sh0118221/18/2022	8:14:2	1	162889	1/12/2022 2:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%			0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1	10	0%			0%	
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985910	B22010507-001	SVOC-8270C-SI	SAMP	V5975.I\sh0118221/18/2022	8:46:4	1	162889	1/12/2022 2:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0196112	0.1	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0167552	0.1	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.0301784	0.1	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.0238	0.1	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.0269416	0.1	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.0258944	0.1	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.0330344	0.1	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.0215152	0.1	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.0254184	0.1	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.028084	0.1	10	0%	0	0	0%	U
Chrysene	A	ug/L	0	0		0	0	0	0.0436016	0.1	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.0349384	0.1	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0	0		0	0	0	0.0221816	0.1	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.02142	0.1	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.0467432	0.1	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.027608	0.1	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.028084	0.1	10	0%	0	0	0%	U
Pyrene	A	ug/L	0	0		0	0	0	0.0227528	0.1	10	0%	0	0	0%	U
1,4-Dichlorobenzene-d4	I	ug/L	40	38.08		0	0	0	0.0952	0.1		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	38.08		0	0	0	0.0952	0.1		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	38.08		0	0	0	0.0952	0.1		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	38.08		0	0	0	0.0952	0.1		0%	0	0	0%	
Perylene-d12	I	ug/L	40	38.08		0	0	0	0.0952	0.1		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	38.08		0	0	0	0.0952	0.1	10	0%	0	0	0%	E
o-Terphenyl	X	ug/L	0	0		190.4	0	0	0.0622608	0	0	0%	40	140	0%	US

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985911	B22010625-001	SVOC-8270C-SI	SAMP	V5975.I\sh0118221/18/2022	9:19:0	1	162889	1/12/2022 2:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.020394	0.1	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.017424	0.1	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.031383	0.1	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.02475	0.1	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.028017	0.1	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.026928	0.1	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.034353	0.1	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.022374	0.1	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.026433	0.1	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.029205	0.1	10	0%	0	0	0%	U
Chrysene	A	ug/L	0	0		0	0	0	0.045342	0.1	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.036333	0.1	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0	0		0	0	0	0.023067	0.1	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.022275	0.1	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.048609	0.1	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.02871	0.1	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.029205	0.1	10	0%	0	0	0%	U
Pyrene	A	ug/L	0	0		0	0	0	0.023661	0.1	10	0%	0	0	0%	U
1,4-Dichlorobenzene-d4	I	ug/L	40	39.6		0	0	0	0.099	0.1		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	39.6		0	0	0	0.099	0.1		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	39.6		0	0	0	0.099	0.1		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	39.6		0	0	0	0.099	0.1		0%	0	0	0%	
Perylene-d12	I	ug/L	40	39.6		0	0	0	0.099	0.1		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	39.6		0	0	0	0.099	0.1	10	0%	0	0	0%	E
o-Terphenyl	X	ug/L	0	0		198	0	0	0.064746	0	0	0%	40	140	0%	US

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985912	B22010626-001	SVOC-8270C-SI	SAMP	V5975.I\sh0118221/18/2022	9:51:1	1	162889	1/12/2022 2:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0198172	0.1	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0169312	0.1	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.0304954	0.1	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.02405	0.1	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.0272246	0.1	10	0%	0	0	0%	U

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985912	B22010626-001	SVOC-8270C-SI	SAMP	V5975.I\sh0118221/18/2022	9:51:1	1	162889	1/12/2022 2:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.0261664	0.1	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.0333814	0.1	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.0217412	0.1	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.0256854	0.1	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.028379	0.1	10	0%	0	0	0%	U
Chrysene	A	ug/L	0	0		0	0	0	0.0440596	0.1	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.0353054	0.1	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0	0		0	0	0	0.0224146	0.1	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.021645	0.1	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.0472342	0.1	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.027898	0.1	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.028379	0.1	10	0%	0	0	0%	U
Pyrene	A	ug/L	0	0		0	0	0	0.0229918	0.1	10	0%	0	0	0%	U
1,4-Dichlorobenzene-d4	I	ug/L	40	38.48		0	0	0	0.0962	0.1		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	38.48		0	0	0	0.0962	0.1		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	38.48		0	0	0	0.0962	0.1		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	38.48		0	0	0	0.0962	0.1		0%	0	0	0%	
Perylene-d12	I	ug/L	40	38.48		0	0	0	0.0962	0.1		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	38.48		0	0	0	0.0962	0.1	10	0%	0	0	0%	E
o-Terphenyl	X	ug/L	0.07981	0.07677722		0	0	0	0.0629148	0	0	0%	40	140	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985913	B22010628-001	SVOC-8270C-SI	SAMP	V5975.I\sh0118221/18/2022	10:23:	1	162889	1/12/2022 2:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0196112	0.1	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0167552	0.1	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.0301784	0.1	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.0238	0.1	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.0269416	0.1	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.0258944	0.1	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.0330344	0.1	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.0215152	0.1	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.0254184	0.1	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.028084	0.1	10	0%	0	0	0%	U

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985913	B22010628-001	SVOC-8270C-SI SAMP		V5975.I\sh0118221/18/2022	10:23:	1	162889	1/12/2022 2:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Chrysene	A	ug/L	0	0		0	0	0	0.0436016	0.1	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.0349384	0.1	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0	0		0	0	0	0.0221816	0.1	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.02142	0.1	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.0467432	0.1	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.027608	0.1	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.028084	0.1	10	0%	0	0	0%	U
Pyrene	A	ug/L	0	0		0	0	0	0.0227528	0.1	10	0%	0	0	0%	U
1,4-Dichlorobenzene-d4	I	ug/L	40	38.08		0	0	0	0.0952	0.1		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	38.08		0	0	0	0.0952	0.1		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	38.08		0	0	0	0.0952	0.1		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	38.08		0	0	0	0.0952	0.1		0%	0	0	0%	
Perylene-d12	I	ug/L	40	38.08		0	0	0	0.0952	0.1		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	38.08		0	0	0	0.0952	0.1	10	0%	0	0	0%	E
o-Terphenyl	X	ug/L	0	0		0	0	0	0.0622608	0	0	0%	40	140	0%	U

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985914	B22010628-001	SVOC-8270C-SI MS-DOD		V5975.I\sh0118221/18/2022	10:55:	1	162889	1/12/2022 2:	1E+07	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	2.92472	2.78433344		4.76	0	0	0.0196112	0.1	10	58%	41	115	0%	
2-Methylnaphthalene	A	ug/L	3.88149	3.69517848		4.76	0	0	0.0167552	0.1	10	78%	39	114	0%	
Acenaphthene	A	ug/L	3.55028	3.37986656		4.76	0	0	0.0301784	0.1	10	71%	48	114	0%	
Acenaphthylene	A	ug/L	3.44286	3.27760272		4.76	0	0	0.0238	0.1	10	69%	35	121	0%	
Anthracene	A	ug/L	4.79468	4.56453536		4.76	0	0	0.0269416	0.1	10	96%	53	119	0%	
Benzo(a)anthracene	A	ug/L	5.09882	4.85407664		4.76	0	0	0.0258944	0.1	10	102%	59	120	0%	
Benzo(a)pyrene	A	ug/L	4.79907	4.56871464		4.76	0	0	0.0330344	0.1	10	96%	53	120	0%	
Benzo(b)fluoranthene	A	ug/L	4.95651	4.71859752		4.76	0	0	0.0215152	0.1	10	99%	53	126	0%	
Benzo(g,h,i)perylene	A	ug/L	4.63272	4.41034944		4.76	0	0	0.0254184	0.1	10	93%	44	128	0%	
Benzo(k)fluoranthene	A	ug/L	4.55488	4.33624576		4.76	0	0	0.028084	0.1	10	91%	54	125	0%	
Chrysene	A	ug/L	4.77015	4.5411828		4.76	0	0	0.0436016	0.1	10	95%	57	120	0%	
Dibenzo(a,h)anthracene	A	ug/L	4.73886	4.51139472		4.76	0	0	0.0349384	0.1	10	95%	44	141	0%	
Fluoranthene	A	ug/L	4.49469	4.27894488		4.76	0	0	0.0221816	0.1	10	90%	58	120	0%	
Fluorene	A	ug/L	4.0712	3.8757824		4.76	0	0	0.02142	0.1	10	81%	50	118	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	4.54416	4.32604032		4.76	0	0	0.0467432	0.1	10	91%	48	130	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985914	B22010628-001	SVOC-8270C-SI	MS-DOD	V5975.I\sh0118221/18/2022	10:55:	1	162889	1/12/2022 2:	1E+07	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Naphthalene	A	ug/L	3.04219	2.89616488		4.76	0	0	0.027608	0.1	10	61%	43	114	0%	
Phenanthrene	A	ug/L	4.73345	4.5062444		4.76	0	0	0.028084	0.1	10	95%	53	115	0%	
Pyrene	A	ug/L	4.56533	4.34619416		4.76	0	0	0.0227528	0.1	10	91%	53	121	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	38.08		0	0	0	0.0952	0.1		0%			0%	
Acenaphthene-d10	I	ug/L	40	38.08		0	0	0	0.0952	0.1		0%			0%	
Chrysene-d12	I	ug/L	40	38.08		0	0	0	0.0952	0.1		0%			0%	
Naphthalene-d8	I	ug/L	40	38.08		0	0	0	0.0952	0.1		0%			0%	
Perylene-d12	I	ug/L	40	38.08		0	0	0	0.0952	0.1		0%			0%	
Phenanthrene-d10	I	ug/L	40	38.08		0	0	0	0.0952	0.1	10	0%			0%	
2-Fluorobiphenyl	S	ug/L	4.40368	4.19230336		4.76	0	0	0.0422688	0.1	10	88%	53	106	0%	
Nitrobenzene-d5	S	ug/L	5.36423	5.10674696		4.76	0	0	0.0497896	0.1	10	107%	55	111	0%	
Terphenyl-d14	S	ug/L	6.76755	6.4427076		4.76	0	0	0.0535976	0.1	10	135%	58	132	0%	S
o-Terphenyl	X	ug/L	4.10834	3.91113968		4.76	0	0	0.0622608	0	0	82%	40	140	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985915	B22010629-001	SVOC-8270C-SI	SAMP	V5975.I\sh0118221/18/2022	11:28:	1	162889	1/12/2022 2:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.021424	0.104	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.018304	0.104	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.032968	0.104	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.026	0.104	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.029432	0.104	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.028288	0.104	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.036088	0.104	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.023504	0.104	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.027768	0.104	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.03068	0.104	10	0%	0	0	0%	U
Chrysene	A	ug/L	0	0		0	0	0	0.047632	0.104	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.038168	0.104	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0	0		0	0	0	0.024232	0.104	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.0234	0.104	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.051064	0.104	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.03016	0.104	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.03068	0.104	10	0%	0	0	0%	U

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985915	B22010629-001	SVOC-8270C-SI	SAMP	V5975.I\sh0118221/18/2022	11:28:	1	162889	1/12/2022 2:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Pyrene	A	ug/L	0	0		0	0	0	0.024856	0.104	10	0%	0	0	0%	U
1,4-Dichlorobenzene-d4	I	ug/L	40	41.6		0	0	0	0.104	0.104		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	41.6		0	0	0	0.104	0.104		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	41.6		0	0	0	0.104	0.104		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	41.6		0	0	0	0.104	0.104		0%	0	0	0%	
Perylene-d12	I	ug/L	40	41.6		0	0	0	0.104	0.104		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	41.6		0	0	0	0.104	0.104	10	0%	0	0	0%	E
o-Terphenyl	X	ug/L	0	0		208	0	0	0.068016	0	0	0%	40	140	0%	US

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985916	B22010633-001	SVOC-8270C-SI	SAMP	V5975.I\sh0118221/19/2022	12:00:	1	162889	1/12/2022 2:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.020188	0.1	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.017248	0.1	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.031066	0.1	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.0245	0.1	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.027734	0.1	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.026656	0.1	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.034006	0.1	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.022148	0.1	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.026166	0.1	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.02891	0.1	10	0%	0	0	0%	U
Chrysene	A	ug/L	0.03379	0		0	0	0	0.044884	0.1	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.035966	0.1	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0.05174	0.0507052		0	0	0	0.022834	0.1	10	0%	0	0	0%	J
Fluorene	A	ug/L	0	0		0	0	0	0.02205	0.1	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.048118	0.1	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.02842	0.1	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.02891	0.1	10	0%	0	0	0%	U
Pyrene	A	ug/L	0.06194	0.0607012		0	0	0	0.023422	0.1	10	0%	0	0	0%	J
1,4-Dichlorobenzene-d4	I	ug/L	40	39.2		0	0	0	0.098	0.1		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	39.2		0	0	0	0.098	0.1		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	39.2		0	0	0	0.098	0.1		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	39.2		0	0	0	0.098	0.1		0%	0	0	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985916	B22010633-001	SVOC-8270C-SI SAMP		V5975.I\sh0118221/19/2022	12:00:	1	162889	1/12/2022 2:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Perylene-d12	I	ug/L	40	39.2		0	0	0	0.098	0.1		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	39.2		0	0	0	0.098	0.1	10	0%	0	0	0%	E
o-Terphenyl	X	ug/L	0	0		196	0	0	0.064092	0	0	0%	40	140	0%	US

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985917	B22010633-001	SVOC-8270C-SI MS-DOD		V5975.I\sh0118221/19/2022	12:32:	1	162889	1/12/2022 2:	1E+07	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	2.69197	2.6650503		4.95	0	0	0.020394	0.1	10	54%	41	115	0%	
2-Methylnaphthalene	A	ug/L	3.41867	3.3844833		4.95	0	0	0.017424	0.1	10	68%	39	114	0%	
Acenaphthene	A	ug/L	3.22653	3.1942647		4.95	0	0	0.031383	0.1	10	65%	48	114	0%	
Acenaphthylene	A	ug/L	3.11949	3.0882951		4.95	0	0	0.02475	0.1	10	62%	35	121	0%	
Anthracene	A	ug/L	4.68988	4.6429812		4.95	0	0	0.028017	0.1	10	94%	53	119	0%	
Benzo(a)anthracene	A	ug/L	5.17075	5.1190425		4.95	0	0	0.026928	0.1	10	103%	59	120	0%	
Benzo(a)pyrene	A	ug/L	4.95995	4.9103505		4.95	0	0	0.034353	0.1	10	99%	53	120	0%	
Benzo(b)fluoranthene	A	ug/L	5.28947	5.2365753		4.95	0	0	0.022374	0.1	10	106%	53	126	0%	
Benzo(g,h,i)perylene	A	ug/L	4.84828	4.7997972		4.95	0	0	0.026433	0.1	10	97%	44	128	0%	
Benzo(k)fluoranthene	A	ug/L	4.69253	4.6456047		4.95	0	0	0.029205	0.1	10	94%	54	125	0%	
Chrysene	A	ug/L	4.76634	4.7186766		4.95	0	0	0.045342	0.1	10	95%	57	120	0%	
Dibenzo(a,h)anthracene	A	ug/L	5.17982	5.1280218		4.95	0	0	0.036333	0.1	10	104%	44	141	0%	
Fluoranthene	A	ug/L	4.46843	4.4237457		4.95	0.0507052	0	0.023067	0.1	10	88%	58	120	0%	
Fluorene	A	ug/L	3.81709	3.7789191		4.95	0	0	0.022275	0.1	10	76%	50	118	0%	
Indeno(1,2,3-cd)pyrene	A	ug/L	4.94451	4.8950649		4.95	0	0	0.048609	0.1	10	99%	48	130	0%	
Naphthalene	A	ug/L	2.67737	2.6505963		4.95	0	0	0.02871	0.1	10	54%	43	114	0%	
Phenanthrene	A	ug/L	4.562	4.51638		4.95	0	0	0.029205	0.1	10	91%	53	115	0%	
Pyrene	A	ug/L	4.68569	4.6388331		4.95	0.0607012	0	0.023661	0.1	10	92%	53	121	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	39.6		0	0	0	0.099	0.1		0%			0%	
Acenaphthene-d10	I	ug/L	40	39.6		0	0	0	0.099	0.1		0%			0%	
Chrysene-d12	I	ug/L	40	39.6		0	0	0	0.099	0.1		0%			0%	
Naphthalene-d8	I	ug/L	40	39.6		0	0	0	0.099	0.1		0%			0%	
Perylene-d12	I	ug/L	40	39.6		0	0	0	0.099	0.1		0%			0%	
Phenanthrene-d10	I	ug/L	40	39.6		0	0	0	0.099	0.1	10	0%			0%	
2-Fluorobiphenyl	S	ug/L	3.98605	3.9461895		4.95	0	0	0.043956	0.1	10	80%	53	106	0%	
Nitrobenzene-d5	S	ug/L	4.72184	4.6746216		4.95	0	0	0.051777	0.1	10	94%	55	111	0%	
Terphenyl-d14	S	ug/L	6.24048	6.1780752		4.95	0	0	0.055737	0.1	10	125%	58	132	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985917	B22010633-001	SVOC-8270C-SI	MS-DOD	V5975.I\sh0118221	19/2022 12:32:	1	162889	1/12/2022 2:	1E+07	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
o-Terphenyl	X	ug/L	4.08718	4.0463082		4.95	0	0	0.064746	0	0	82%	40	140	0%	
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985918	B22010637-001	SVOC-8270C-SI	SAMP	V5975.I\sh0118221	19/2022 1:04:5	1	162889	1/12/2022 2:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0206	0.1	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0176	0.1	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.0317	0.1	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.025	0.1	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.0283	0.1	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.0272	0.1	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.0347	0.1	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.0226	0.1	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.0267	0.1	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.0295	0.1	10	0%	0	0	0%	U
Chrysene	A	ug/L	0	0		0	0	0	0.0458	0.1	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.0367	0.1	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0	0		0	0	0	0.0233	0.1	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.0225	0.1	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.0491	0.1	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.029	0.1	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.0295	0.1	10	0%	0	0	0%	U
Pyrene	A	ug/L	0	0		0	0	0	0.0239	0.1	10	0%	0	0	0%	U
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1	10	0%	0	0	0%	E
o-Terphenyl	X	ug/L	0.05257	0		0	0	0	0.0654	0	0	0%	40	140	0%	U

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985919	B22010641-001	SVOC-8270C-SI	SAMP	V5975.I\sh0118221/19/2022	1:37:0	1	162889	1/12/2022 2:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0200026	0.1	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0170896	0.1	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.0307807	0.1	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.024275	0.1	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.0274793	0.1	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.0264112	0.1	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.0336937	0.1	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.0219446	0.1	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.0259257	0.1	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.0286445	0.1	10	0%	0	0	0%	U
Chrysene	A	ug/L	0	0		0	0	0	0.0444718	0.1	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.0356357	0.1	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0	0		0	0	0	0.0226243	0.1	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.0218475	0.1	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.0476761	0.1	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.028159	0.1	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.0286445	0.1	10	0%	0	0	0%	U
Pyrene	A	ug/L	0	0		0	0	0	0.0232069	0.1	10	0%	0	0	0%	U
1,4-Dichlorobenzene-d4	I	ug/L	40	38.84		0	0	0	0.0971	0.1		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	38.84		0	0	0	0.0971	0.1		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	38.84		0	0	0	0.0971	0.1		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	38.84		0	0	0	0.0971	0.1		0%	0	0	0%	
Perylene-d12	I	ug/L	40	38.84		0	0	0	0.0971	0.1		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	38.84		0	0	0	0.0971	0.1	10	0%	0	0	0%	E
o-Terphenyl	X	ug/L	0	0		4.855	0	0	0.0635034	0	0	0%	40	140	0%	US

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985920	B22010643-001	SVOC-8270C-SI	SAMP	V5975.I\sh0118221/19/2022	2:09:1	1	162889	1/12/2022 2:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0200026	0.1	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.0170896	0.1	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.0307807	0.1	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.024275	0.1	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.0274793	0.1	10	0%	0	0	0%	U

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985920	B22010643-001	SVOC-8270C-SI	SAMP	V5975.I\sh0118221/19/2022	2:09:1	1	162889	1/12/2022 2:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.0264112	0.1	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.0336937	0.1	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.0219446	0.1	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.0259257	0.1	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.0286445	0.1	10	0%	0	0	0%	U
Chrysene	A	ug/L	0	0		0	0	0	0.0444718	0.1	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.0356357	0.1	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0	0		0	0	0	0.0226243	0.1	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.0218475	0.1	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.0476761	0.1	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.028159	0.1	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.0286445	0.1	10	0%	0	0	0%	U
Pyrene	A	ug/L	0	0		0	0	0	0.0232069	0.1	10	0%	0	0	0%	U
1,4-Dichlorobenzene-d4	I	ug/L	40	38.84		0	0	0	0.0971	0.1		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	38.84		0	0	0	0.0971	0.1		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	38.84		0	0	0	0.0971	0.1		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	38.84		0	0	0	0.0971	0.1		0%	0	0	0%	
Perylene-d12	I	ug/L	40	38.84		0	0	0	0.0971	0.1		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	38.84		0	0	0	0.0971	0.1	10	0%	0	0	0%	E
o-Terphenyl	X	ug/L	0	0		194.2	0	0	0.0635034	0	0	0%	40	140	0%	US

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985921	B22010643-002	SVOC-8270C-SI	SAMP	V5975.I\sh0118221/19/2022	2:41:3	1	162889	1/12/2022 2:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.020188	0.1	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.017248	0.1	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.031066	0.1	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.0245	0.1	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.027734	0.1	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0	0		0	0	0	0.026656	0.1	10	0%	0	0	0%	U
Benzo(a)pyrene	A	ug/L	0	0		0	0	0	0.034006	0.1	10	0%	0	0	0%	U
Benzo(b)fluoranthene	A	ug/L	0	0		0	0	0	0.022148	0.1	10	0%	0	0	0%	U
Benzo(g,h,i)perylene	A	ug/L	0	0		0	0	0	0.026166	0.1	10	0%	0	0	0%	U
Benzo(k)fluoranthene	A	ug/L	0	0		0	0	0	0.02891	0.1	10	0%	0	0	0%	U

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985921	B22010643-002	SVOC-8270C-SI	SAMP	V5975.I\sh0118221	19/2022 2:41:3	1	162889	1/12/2022 2:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Chrysene	A	ug/L	0	0		0	0	0	0.044884	0.1	10	0%	0	0	0%	U
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.035966	0.1	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0	0		0	0	0	0.022834	0.1	10	0%	0	0	0%	U
Fluorene	A	ug/L	0	0		0	0	0	0.02205	0.1	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0	0		0	0	0	0.048118	0.1	10	0%	0	0	0%	U
Naphthalene	A	ug/L	0	0		0	0	0	0.02842	0.1	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.02891	0.1	10	0%	0	0	0%	U
Pyrene	A	ug/L	0	0		0	0	0	0.023422	0.1	10	0%	0	0	0%	U
1,4-Dichlorobenzene-d4	I	ug/L	40	39.2		0	0	0	0.098	0.1		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	39.2		0	0	0	0.098	0.1		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	39.2		0	0	0	0.098	0.1		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	39.2		0	0	0	0.098	0.1		0%	0	0	0%	
Perylene-d12	I	ug/L	40	39.2		0	0	0	0.098	0.1		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	39.2		0	0	0	0.098	0.1	10	0%	0	0	0%	E
o-Terphenyl	X	ug/L	0.13196	0.1293208		196	0	0	0.064092	0	0	0%	40	140	0%	S

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985922	B22010751-001	SVOC-8270C-SI	SAMP	V5975.I\sh0118221	19/2022 3:13:5	1	162889	1/13/2022 1	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
1-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.020806	0.101	10	0%	0	0	0%	U
2-Methylnaphthalene	A	ug/L	0	0		0	0	0	0.017776	0.101	10	0%	0	0	0%	U
Acenaphthene	A	ug/L	0	0		0	0	0	0.032017	0.101	10	0%	0	0	0%	U
Acenaphthylene	A	ug/L	0	0		0	0	0	0.02525	0.101	10	0%	0	0	0%	U
Anthracene	A	ug/L	0	0		0	0	0	0.028583	0.101	10	0%	0	0	0%	U
Benzo(a)anthracene	A	ug/L	0.1591	0.160691		0	0	0	0.027472	0.101	10	0%	0	0	0%	
Benzo(a)pyrene	A	ug/L	0.12544	0.1266944		0	0	0	0.035047	0.101	10	0%	0	0	0%	
Benzo(b)fluoranthene	A	ug/L	0.19347	0.1954047		0	0	0	0.022826	0.101	10	0%	0	0	0%	
Benzo(g,h,i)perylene	A	ug/L	0.08586	0.0867186		0	0	0	0.026967	0.101	10	0%	0	0	0%	J
Benzo(k)fluoranthene	A	ug/L	0.07468	0.0754268		0	0	0	0.029795	0.101	10	0%	0	0	0%	J
Chrysene	A	ug/L	0.15448	0.1560248		0	0	0	0.046258	0.101	10	0%	0	0	0%	
Dibenzo(a,h)anthracene	A	ug/L	0	0		0	0	0	0.037067	0.101	10	0%	0	0	0%	U
Fluoranthene	A	ug/L	0.13531	0.1366631		0	0	0	0.023533	0.101	10	0%	0	0	0%	
Fluorene	A	ug/L	0	0		0	0	0	0.022725	0.101	10	0%	0	0	0%	U
Indeno(1,2,3-cd)pyrene	A	ug/L	0.10536	0.1064136		0	0	0	0.049591	0.101	10	0%	0	0	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985922	B22010751-001	SVOC-8270C-SI	SAMP	V5975.I\sh0118221	19/2022 3:13:5	1	162889	1/13/2022	1	0	0					
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Naphthalene	A	ug/L	0	0		0	0	0	0.02929	0.101	10	0%	0	0	0%	U
Phenanthrene	A	ug/L	0	0		0	0	0	0.029795	0.101	10	0%	0	0	0%	U
Pyrene	A	ug/L	0.26853	0.2712153		0	0	0	0.024139	0.101	10	0%	0	0	0%	
1,4-Dichlorobenzene-d4	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%	0	0	0%	
Acenaphthene-d10	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%	0	0	0%	
Chrysene-d12	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%	0	0	0%	
Naphthalene-d8	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%	0	0	0%	
Perylene-d12	I	ug/L	40	40.4		0	0	0	0.101	0.101		0%	0	0	0%	
Phenanthrene-d10	I	ug/L	40	40.4		0	0	0	0.101	0.101	10	0%	0	0	0%	E
o-Terphenyl	X	ug/L	0	0		202	0	0	0.066054	0	0	0%	40	140	0%	US

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist						
14985923	18-Jan-22_CCV	SVOC-8270C-SI	CCV	V5975.I\sh0118221	19/2022 3:46:0	1	R373371				0	0					
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q	
1-Methylnaphthalene	A	ug/L	1.79101	1.79101		2	0	0	0.0206	0.1	10	90%	50	150	0%		
2-Methylnaphthalene	A	ug/L	1.95472	1.95472		2	0	0	0.0176	0.1	10	98%	50	150	0%		
Acenaphthene	A	ug/L	1.66668	1.66668		2	0	0	0.0317	0.1	10	83%	50	150	0%		
Acenaphthylene	A	ug/L	1.62025	1.62025		2	0	0	0.025	0.1	10	81%	50	150	0%		
Anthracene	A	ug/L	2.05903	2.05903		2	0	0	0.0283	0.1	10	103%	50	150	0%		
Benzo(a)anthracene	A	ug/L	2.01835	2.01835		2	0	0	0.0272	0.1	10	101%	50	150	0%		
Benzo(a)pyrene	A	ug/L	2.01194	2.01194		2	0	0	0.0347	0.1	10	101%	50	150	0%		
Benzo(b)fluoranthene	A	ug/L	1.91413	1.91413		2	0	0	0.0226	0.1	10	96%	50	150	0%		
Benzo(g,h,i)perylene	A	ug/L	1.88155	1.88155		2	0	0	0.0267	0.1	10	94%	50	150	0%		
Benzo(k)fluoranthene	A	ug/L	1.82405	1.82405		2	0	0	0.0295	0.1	10	91%	50	150	0%		
Chrysene	A	ug/L	1.90186	1.90186		2	0	0	0.0458	0.1	10	95%	50	150	0%		
Dibenzo(a,h)anthracene	A	ug/L	1.78271	1.78271		2	0	0	0.0367	0.1	10	89%	50	150	0%		
Fluoranthene	A	ug/L	1.86845	1.86845		2	0	0	0.0233	0.1	10	93%	50	150	0%		
Fluorene	A	ug/L	1.74968	1.74968		2	0	0	0.0225	0.1	10	87%	50	150	0%		
Indeno(1,2,3-cd)pyrene	A	ug/L	2.04547	2.04547		2	0	0	0.0491	0.1	10	102%	50	150	0%		
Naphthalene	A	ug/L	1.76934	1.76934		2	0	0	0.029	0.1	10	88%	50	150	0%		
Phenanthrene	A	ug/L	1.98875	1.98875		2	0	0	0.0295	0.1	10	99%	50	150	0%		
Pyrene	A	ug/L	1.83489	1.83489		2	0	0	0.0239	0.1	10	92%	50	150	0%		
1,4-Dichlorobenzene-d4	I	ug/L	40	40		0	0	0	0.1	0.1		0%	50	150	0%		
Acenaphthene-d10	I	ug/L	40	40		0	0	0	0.1	0.1		0%	50	150	0%		

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14985923	18-Jan-22_CCV	SVOC-8270C-SI	CCV	V5975.I\sh0118221/19/2022	3:46:0	1	R373371		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Chrysene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	50	150	0%	
Naphthalene-d8	I	ug/L	40	40		0	0	0	0.1	0.1		0%	50	150	0%	
Perylene-d12	I	ug/L	40	40		0	0	0	0.1	0.1		0%	50	150	0%	
Phenanthrene-d10	I	ug/L	40	40		0	0	0	0.1	0.1	10	0%	50	150	0%	
2-Fluorobiphenyl	S	ug/L	1.64504	1.64504		2	0	0	0.0444	0.1	10	82%	50	150	0%	
Nitrobenzene-d5	S	ug/L	2.11436	2.11436		2	0	0	0.0523	0.1	10	106%	50	150	0%	
Terphenyl-d14	S	ug/L	1.98815	1.98815		2	0	0	0.0563	0.1	10	99%	50	150	0%	
o-Terphenyl	X	ug/L	1.80357	1.80357		2	0	0	0.0654	0	0	90%	50	150	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14986414	LLCS-162800	SVOC-8270-W-	LCS-DOD	V5975.I\sh0118221/18/2022	6:05:1	20	162800	1/10/2022 8:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
2-Fluorobiphenyl	S	ug/L	3.72314	74.4628		100	0	0	0.888	2	0	74%	53	106	0%	
Nitrobenzene-d5	S	ug/L	3.92807	78.5614		100	0	0	1.046	2	0	79%	55	111	0%	
Terphenyl-d14	S	ug/L	6.05682	121.1364		100	0	0	1.126	2	0	121%	58	132	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14986415	LLCSD-162800	SVOC-8270-W-	LCSD-DOD	V5975.I\sh0118221/18/2022	6:37:2	1	162800	1/10/2022 8:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
2-Fluorobiphenyl	S	ug/L	3.24675	3.24675		5	0	0	0.0444	0.1	0	65%	53	106	0%	
Nitrobenzene-d5	S	ug/L	4.39731	4.39731		5	0	0	0.0523	0.1	0	88%	55	111	0%	
Terphenyl-d14	S	ug/L	5.52495	5.52495		5	0	0	0.0563	0.1	0	110%	58	132	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14986416	LLCS-162889	SVOC-8270-W-	LCS-DOD	V5975.I\sh0118221/18/2022	7:09:4	1	162889	1/12/2022 2:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
2-Fluorobiphenyl	S	ug/L	3.39211	3.39211		5	0	0	0.0444	0.1	0	68%	53	106	0%	
Nitrobenzene-d5	S	ug/L	4.06312	4.06312		5	0	0	0.0523	0.1	0	81%	55	111	0%	
Terphenyl-d14	S	ug/L	5.05279	5.05279		5	0	0	0.0563	0.1	0	101%	58	132	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14986417	LLCSD-162889	SVOC-8270-W-	LCSD-DOD	V5975.I\sh0118221	18/2022 7:42:0	1	162889	1/12/2022 2:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
2-Fluorobiphenyl	S	ug/L	3.06148	3.06148		5	0	0	0.0444	0.1	0	61%	53	106	0%	
Nitrobenzene-d5	S	ug/L	3.87605	3.87605		5	0	0	0.0523	0.1	0	78%	55	111	0%	
Terphenyl-d14	S	ug/L	5.07681	5.07681		5	0	0	0.0563	0.1	0	102%	58	132	0%	
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14986418	B22010628-001	SVOC-8270-W-	MS-DOD	V5975.I\sh0118221	18/2022 10:55:	1	162889	1/12/2022 2:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
2-Fluorobiphenyl	S	ug/L	4.40368	4.19230336		4.76	0	0	0.0422688	0.1	0	88%	53	106	0%	
Nitrobenzene-d5	S	ug/L	5.36423	5.10674696		4.76	0	0	0.0497896	0.1	0	107%	55	111	0%	
Terphenyl-d14	S	ug/L	6.76755	6.4427076		4.76	0	0	0.0535976	0.1	0	135%	58	132	0%	S
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14986419	B22010633-001	SVOC-8270-W-	MS-DOD	V5975.I\sh0118221	19/2022 12:32:	1	162889	1/12/2022 2:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
2-Fluorobiphenyl	S	ug/L	3.98605	3.9461895		4.95	0	0	0.043956	0.1	0	80%	53	106	0%	
Nitrobenzene-d5	S	ug/L	4.72184	4.6746216		4.95	0	0	0.051777	0.1	0	94%	55	111	0%	
Terphenyl-d14	S	ug/L	6.24048	6.1780752		4.95	0	0	0.055737	0.1	0	125%	58	132	0%	



Write Sequence

Insert Entries(Have the first cell for entries selected)

File Name	Sample Name	Line No.	Test Code	Multiplier	Divisor	Method Name
Jan1801.d	18-Jan-22_TUNE_1	1		1	1	5975Tune.M
Jan1802.d	18-Jan-22_CCV_2	2	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1803.d	18-Jan-22_ISTBLK_3	3	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1804.d	B22010212-001C	4	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1805.d	B22010211-001C	5	SVOC-8270C-SIM-W-LLPA	100	1	5975BNASIM.M
Jan1806.d	LLCS-162800	6	SVOC-8270C-SIM-W-LLPA	20	1	5975BNASIM.M
Jan1807.d	LLCSD-162800	7	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1808.d	LLCS-162889	8	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1809.d	LLCSD-162889	9	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1810.d	MB-162889	10	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1811.d	B22010507-001C	11	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1812.d	B22010625-001C	12	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1813.d	B22010626-001C	13	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1814.d	B22010628-001C	14	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1815.d	B22010628-001CLMS	15	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1816.d	B22010629-001C	16	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1817.d	B22010633-001C	17	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1818.d	B22010633-001CLMS	18	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1819.d	B22010637-001C	19	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1820.d	B22010641-001C	20	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1821.d	B22010643-001C	21	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1822.d	B22010643-002A	22	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1823.d	B22010751-001C	23	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1824.d	18-Jan-22_CCV_24	24	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1825.d	18-Jan-22_TUNE_25	25		1	1	5975Tune.M
Jan1826.d	18-Jan-22_CCV_26	26	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1827.d	18-Jan-22_ISTBLK_27	27	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1828.d	MB-162956	28	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1829.d	LLCS-162956	29	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1830.d	LLCSD-162956	30	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1831.d	B22010753-001C	31	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1832.d	B22010754-001C	32	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1833.d	B22010750-001C	33	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1834.d	B22010755-001C	34	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1835.d	B22010756-001C	35	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1836.d	B22010757-001C	36	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1837.d	B22010758-001C	37	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1838.d	B22010758-002A	38	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1839.d	B22010759-001C	39	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1840.d	B22010759-001CLMS	40	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1841.d	B22010759-001CLMSD	41	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M
Jan1842.d	18-Jan-22_CCV_42	42	SVOC-8270C-SIM-W-LLPA	1	1	5975BNASIM.M









Tune Evaluation Report

Data Path: \\MASSHUNTER\Org\Data\SV5975.I\sh011822\1 e8270c bna SIMJan1801.D
 Acq on: 1/18/2022 3:31:39 PM
 Operator: LIMS import
 Sample: 18-Jan-22_TUNE_1
 Inst Name: GCMS
 ALS Vial: 1
 Method: \\MASSHUNTER\Org\Data\SV5975.I\Methods\DFTPP5975625.m




Target Mass	Rel. To Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Pass/Fail
51	198	30	60	46.9	123704	Pass
68	69	0	2	0.0	0	Pass
70	69	0	2	0.6	1145	Pass
127	198	40	60	59.6	157120	Pass
197	198	0	1	0.0	0	Pass
198	198	100	100	100.0	263616	Pass
199	198	5	9	7.2	19000	Pass
275	198	10	30	26.7	70488	Pass
365	198	1	100	3.2	8398	Pass
441	443	1E-10	150	89.0	29984	Pass
442	198	40	100	66.6	175680	Pass
443	442	17	23	19.2	33696	Pass
69	69	100	100	100.0	191296	Pass

Tune Evaluation Report



Tune Evaluation Report


+ Scan (rt: 8.181-8.220 min, 28 scans) Jan1801.D 4,4'-DDE




Compound Name	Expected RT	Observed RT	TIC Area	Breakdown %	Pass/Fail
4,4'-DDT	8.800	8.701	3321272	0.0	Pass
4,4'-DDD	8.500	0.000	0		
4,4'-DDE	8.200	0.000	0		

Tune Evaluation Report

+ Scan (rt: 6.396 min) Jan1801.D Pentachlorophenol



+ Scan (rt: 7.923 min) Jan1801.D Benzidine




Compound Name	Expected RT	Observed RT	Tailing Factor	PGF	Pass/Fail
Pentachlorophenol	6.800	6.396	0.5	3.6	Pass
Benzidine	8.400	7.923	0.2	2.5	Pass

Quantitation Results Report (QT Reviewed)

Data File	Jan1802.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/18/2022 3:55:24 PM
Sample Name	18-Jan-22_CCV_2	Instrument	GCMS
Vial	2	Multiplier	1.00
DA Method File	011722 bna SIM 1.batch.bin	Comment	SVOC-8270C-SIM-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011822 bna SIM1.batch.bin	Last Calib Update	1/17/2022 8:49:06 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.484	152.0	185938	40.0000	ng/ml	-0.012
M Naphthalene-d8	5.928	136.0	338631	40.0000	ng/ml	-0.012
M Acenaphthene-d10	8.000	164.0	186457	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.768	188.0	381095	40.0000	ng/ml	-0.012
M Chrysene-d12	14.714	240.0	260043	40.0000	ng/ml	-0.012
M Perylene-d12	18.487	264.0	176150	40.0000	ng/ml	-0.012
System Monitoring Compounds						
S Nitrobenzene-d5	5.131	82.0	6464	1.8340	ng/ml	-0.012
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 36.68%		
S 2-Fluorobiphenyl	7.252	172.0	17435	1.9453	ng/ml	-0.012
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 38.91%		
S o-Terphenyl	10.299	230.0	11336	1.8276	ng/ml	0.000
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = 36.55%		*
S Terphenyl-d14	12.251	244.0	9862	2.0599	ng/ml	-0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 41.20%		
Target Compounds						
T Naphthalene	5.953	128.0	19528	1.6668	ng/ml	98
T 2-Methylnaphthalene	6.777	141.0	12456	1.9049	ng/ml	99
T 1-Methylnaphthalene	6.890	141.0	12713	1.8435	ng/ml	95
T Acenaphthylene	7.826	152.0	20515	1.7953	ng/ml	m 98
T Acenaphthene	8.038	154.0	12452	1.7036	ng/ml	93
T Fluorene	8.661	166.0	15973	1.8468	ng/ml	98
T Phenanthrene	9.793	178.0	22717	1.9307	ng/ml	94
T Anthracene	9.854	178.0	20676	2.0129	ng/ml	100
T Fluoranthene	11.411	202.0	23235	1.7977	ng/ml	99
T Pyrene	11.781	202.0	26272	2.0055	ng/ml	99
T Benzo(a)Anthracene	14.677	228.0	17533	2.1225	ng/ml	99
T Chrysene	14.776	228.0	21859	1.8366	ng/ml	96
T Benzo(b)fluoranthene	17.708	252.0	14536	1.8317	ng/ml	98


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	17.783	252.0	17953	1.9817	ng/ml	98
T Benzo(a)pyrene	18.363	252.0	12777	2.1113	ng/ml	98
T Indeno(1,2,3-cd)pyrene	20.204	276.0	11564	2.0061	ng/ml	100
T Dibenzo(a,h)anthracene	20.278	278.0	12813	1.8208	ng/ml	98
T Benzo(g,h,i)perylene	20.538	276.0	16337	1.9494	ng/ml	97


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	1.8340	5.13	-0.01	6464	54.0	38.4	25.9	48.1
					128.0	40.1	25.6	47.6



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	1.6668	5.95	0.00	19528	102.0	21.6	0.0	59.6
					129.0	11.0	7.7	14.3




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	1.9049	6.78	-0.01	12456	142.0	139.1	98.5	183.0
					115.0	58.9	41.8	77.6




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	1.8435	6.89	-0.01	12713	142.0	116.1	79.2	147.1
					115.0	60.9	47.5	88.2




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	1.9453	7.25	-0.01	17435	171.0	35.6	26.6	49.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthylene	1.7953	7.83	0.00	20515 (m)	153.0	13.5	9.0	16.6






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	1.7036	8.04	0.00	12452	153.0	108.2	82.1	152.6
					152.0	54.5	41.0	76.1






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene	1.8468	8.66	-0.01	15973	165.0	101.0	69.1	128.3
					167.0	13.3	9.7	18.0






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Phenanthrene	1.9307	9.79	-0.01	22717	176.0	18.1	10.8	20.1



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Anthracene	2.0129	9.85	-0.01	20676	176.0	18.1	12.7	23.5




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
o-Terphenyl	1.8276	10.30	0.00	11336	229.0	68.5	49.2	91.3
					215.0	45.6	32.7	60.7




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluoranthene	1.7977	11.41	0.00	23235	101.0	13.5	9.6	17.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Pyrene	2.0055	11.78	-0.01	26272	101.0	14.9	10.7	20.0















Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	2.0599	12.25	-0.01	9862	122.0	18.6	13.4	25.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)Anthracene	2.1225	14.68	-0.02	17533	226.0	26.4	18.9	35.1
					229.0	22.2	16.1	29.9



Quantitation Results Report (QT Reviewed)

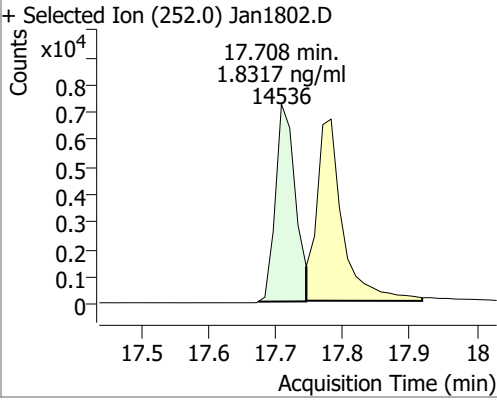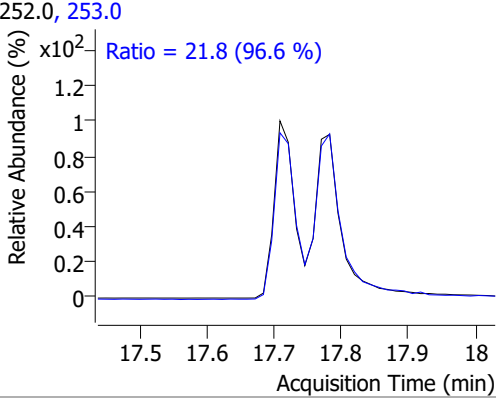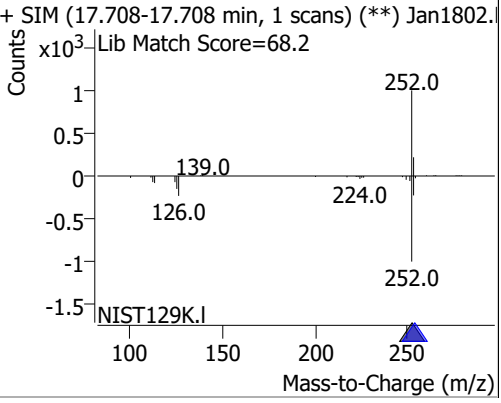Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	1.8366	14.78	-0.01	21859	226.0 229.0	31.8 18.8	21.2 15.0	39.4 27.8
+ Selected Ion (228.0) Jan1802.D 			228.0, 226.0, 229.0 			+ SIM (14.776-14.776 min, 1 scans) (**) Jan1802.D Lib Match Score=55.0 		
Benzo(b)fluoranthene	1.8317	17.71	-0.02	14536	253.0	21.8	15.8	29.4
+ Selected Ion (252.0) Jan1802.D 			252.0, 253.0 			+ SIM (17.708-17.708 min, 1 scans) (**) Jan1802.D Lib Match Score=68.2 		
Benzo(k)fluoranthene	1.9817	17.78	-0.01	17953	253.0	23.7	16.1	29.9
+ Selected Ion (252.0) Jan1802.D 			252.0, 253.0 			+ SIM (17.783-17.783 min, 1 scans) (**) Jan1802.D Lib Match Score=68.1 		
Benzo(a)pyrene	2.1113	18.36	-0.01	12777	253.0	22.7	16.5	30.6
+ Selected Ion (252.0) Jan1802.D 			252.0, 253.0 			+ SIM (18.363-18.363 min, 1 scans) (**) Jan1802.D Lib Match Score=68.2 		


Quantitation Results Report (QT Reviewed)

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Indeno(1,2,3-cd)pyrene	2.0061	20.20	-0.02	11564	138.0	29.1	20.3	37.6
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1802.D</p> </div> <div style="width: 30%;"> <p>276.0, 138.0</p> <p>Ratio = 29.1 (100.5 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.204-20.204 min, 1 scans) (**) Jan1802.D</p> <p>Lib Match Score=75.9</p> </div> </div>								
Dibenzo(a,h)anthracene	1.8208	20.28	-0.02	12813	279.0	24.7	17.6	32.7
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (278.0) Jan1802.D</p> </div> <div style="width: 30%;"> <p>278.0, 279.0, 139.0</p> <p>Ratio = 24.7 (98.2 %)</p> <p>Ratio = 22.4 (92.9 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.278-20.278 min, 1 scans) (**) Jan1802.D</p> <p>Lib Match Score=75.6</p> </div> </div>								
Benzo(g,h,i)perylene	1.9494	20.54	-0.02	16337	138.0	26.1	19.6	36.5
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1802.D</p> </div> <div style="width: 30%;"> <p>276.0, 138.0, 277.0</p> <p>Ratio = 26.1 (93.0 %)</p> <p>Ratio = 24.3 (104.7 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.538-20.538 min, 1 scans) (**) Jan1802.D</p> <p>Lib Match Score=75.8</p> </div> </div>								

Quantitation Results Report (QT Reviewed)

Data File	Jan1803.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/18/2022 4:27:47 PM
Sample Name	18-Jan-22_ISTBLK_3	Instrument	GCMS
Vial	3	Multiplier	1.00
DA Method File	011722 bna SIM 1.batch.bin	Comment	SVOC-8270C-SIM-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011822 bna SIM1.batch.bin	Last Calib Update	1/17/2022 8:49:06 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)	
Internal Standards							
M 1,4-Dichlorobenzene-d4	4.484	152.0	183041	40.0000	ng/ml	-0.012	
M Naphthalene-d8	5.928	136.0	319600	40.0000	ng/ml	-0.012	
M Acenaphthene-d10	8.000	164.0	187792	40.0000	ng/ml	0.000	
M Phenanthrene-d10	9.768	188.0	373785	40.0000	ng/ml	-0.012	
M Chrysene-d12	14.714	240.0	251166	40.0000	ng/ml	-0.012	
M Perylene-d12	18.475	264.0	168890	40.0000	ng/ml	-0.025	
System Monitoring Compounds							
S Nitrobenzene-d5	0.000		0	N.D.			
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = NA%			
S 2-Fluorobiphenyl	0.000		0	N.D.			
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = NA%			
S o-Terphenyl	0.000		0	N.D.			
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%			
S Terphenyl-d14	0.000		0	N.D.			
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = NA%			
Target Compounds							
T Naphthalene	0.000		0	N.D.			QValue
T 2-Methylnaphthalene	0.000		0	N.D.			
T 1-Methylnaphthalene	0.000		0	N.D.			
T Acenaphthylene	0.000		0	N.D.			
T Acenaphthene	8.013	154.0	0		ng/ml md		1
T Fluorene	0.000		0	N.D.			
T Phenanthrene	0.000		0	N.D.			
T Anthracene	0.000		0	N.D.			
T Fluoranthene	0.000		0	N.D.			
T Pyrene	0.000		0	N.D.			
T Benzo(a)Anthracene	14.701	228.0	0		ng/ml md		1
T Chrysene	14.776	228.0	0		ng/ml md		1
T Benzo(b)fluoranthene	0.000		0	N.D.			


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.363	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Nitrobenzene-d5	N.D.	5.14	54.0	37.0	128.0	36.6




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.95	102.0	19.9	129.0	11.0



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.79	142.0	140.8	115.0	59.7




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	113.1	115.0	67.8




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
2-Fluorobiphenyl	N.D.	7.26	171.0	38.0




Compound	Conc.	Exp RT	QIon	Exp Ratio
Acenaphthylene	N.D.	7.83	153.0	12.8











Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene		0		0	153.0		82.1	152.6
					152.0		41.0	76.1







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Fluorene	N.D.	8.67	165.0	98.7	167.0	13.8







Quantitation Results Report (QT Reviewed)

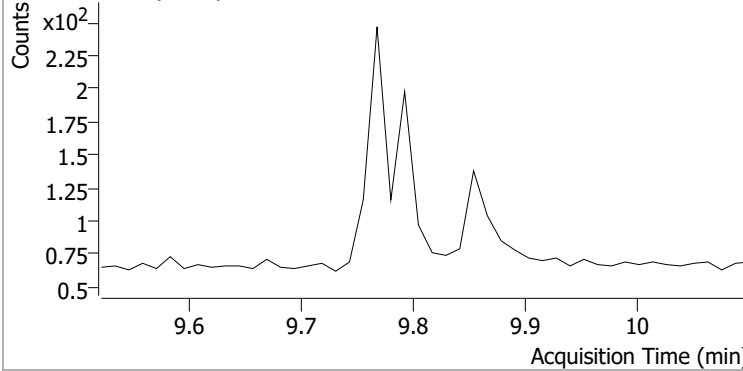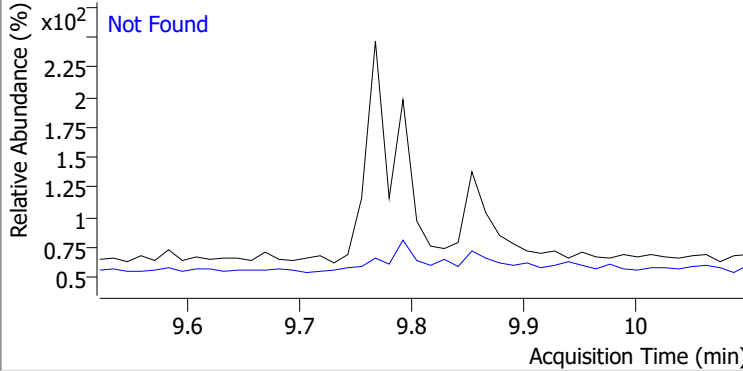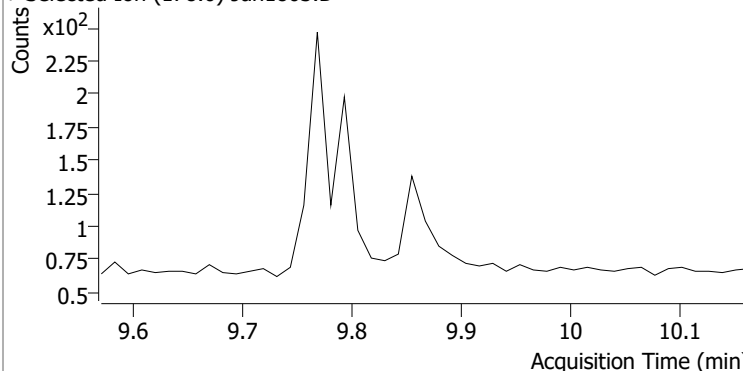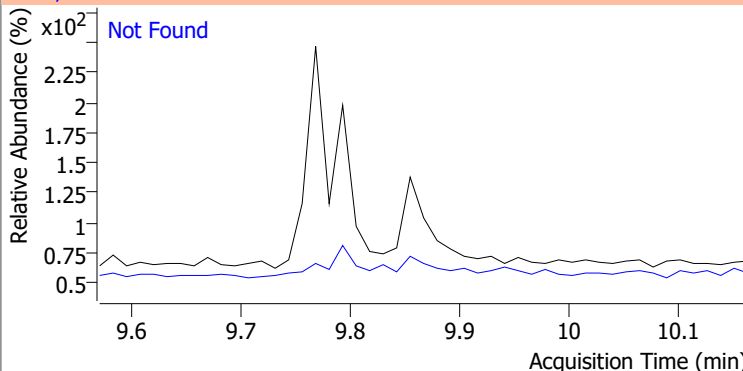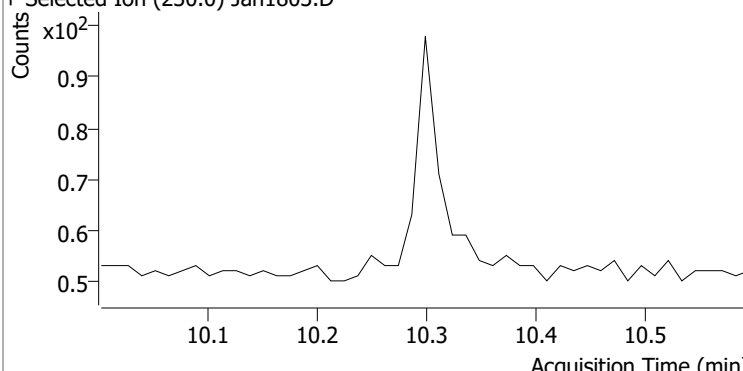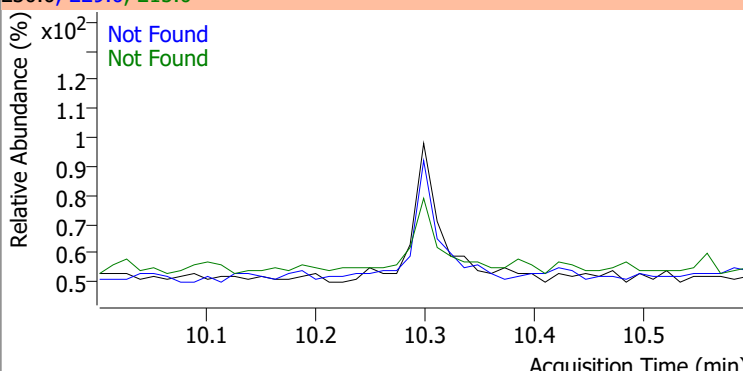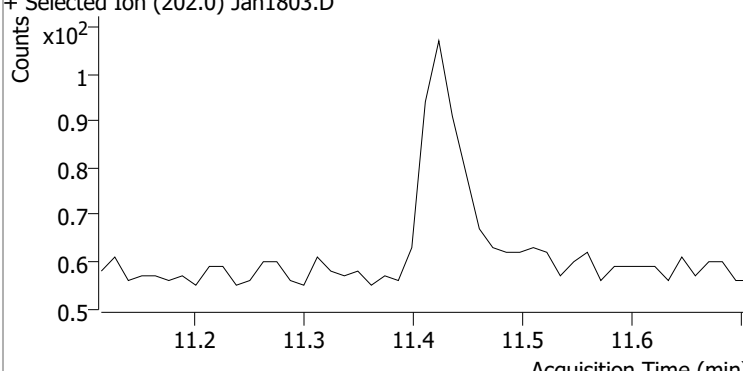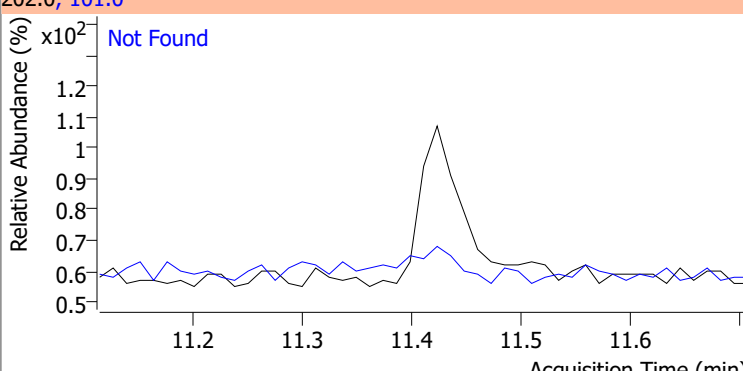Compound	Conc.	Exp RT	QIon	Exp Ratio		
Phenanthrene	N.D.	9.80	176.0	15.5		
+ Selected Ion (178.0) Jan1803.D			178.0, 176.0			
						
Anthracene	N.D.	9.87	176.0	18.1		
+ Selected Ion (178.0) Jan1803.D			178.0, 176.0			
						
o-Terphenyl	N.D.	10.30	229.0	70.2	QIon	Exp Ratio
+ Selected Ion (230.0) Jan1803.D			230.0, 229.0, 215.0			
						
Fluoranthene	N.D.	11.41	101.0	13.8		
+ Selected Ion (202.0) Jan1803.D			202.0, 101.0			
						

Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)

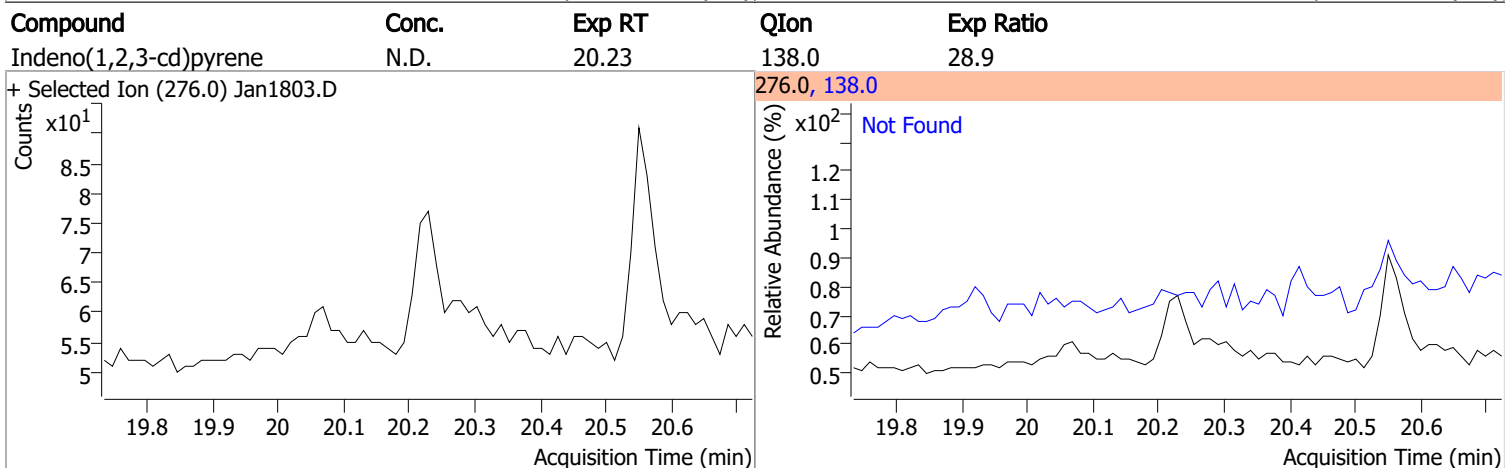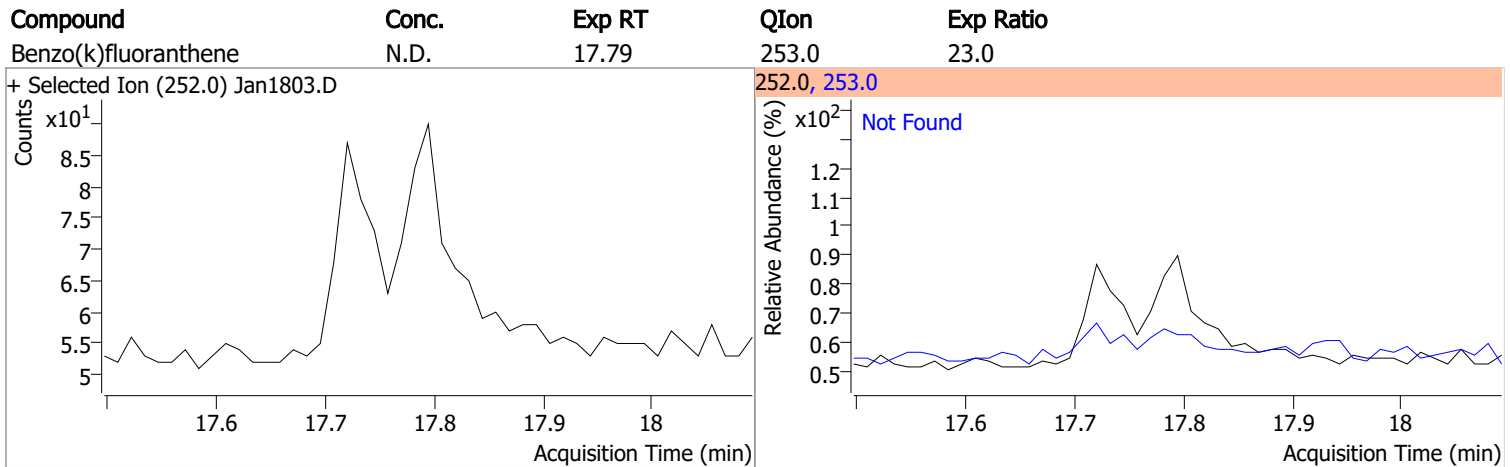


Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.30	279.0	25.1	139.0	24.1




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.56	138.0	28.0	277.0	23.3



Quantitation Results Report (QT Reviewed)

Data File	Jan1804.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/18/2022 5:00:17 PM
Sample Name	B22010212-001C	Instrument	GCMS
Vial	4	Multiplier	1.00
DA Method File	011722 bna SIM 1.batch.bin	Comment	SVOC-8270C-SIM-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011822 bna SIM1.batch.bin	Last Calib Update	1/17/2022 8:49:06 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.484	152.0	184453	40.0000	ng/ml	-0.012
M Naphthalene-d8	5.928	136.0	338164	40.0000	ng/ml	-0.012
M Acenaphthene-d10	8.001	164.0	188772	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.768	188.0	363168	40.0000	ng/ml	-0.012
M Chrysene-d12	14.714	240.0	253149	40.0000	ng/ml	-0.012
M Perylene-d12	18.475	264.0	169801	40.0000	ng/ml	-0.025
System Monitoring Compounds						
S Nitrobenzene-d5	5.118	82.0	347267	35.7347	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 714.69%		*
S 2-Fluorobiphenyl	7.252	172.0	522576	57.5926	ng/ml	-0.012
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1151.85%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.251	244.0	512340	75.1285	ng/ml	-0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 1502.57%		*
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.001	154.0	0		ng/ml	md
T Fluorene	8.661	166.0	0		ng/ml	md
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.702	228.0	0		ng/ml	md
T Chrysene	14.702	228.0	0		ng/ml	md
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.475	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	35.7347	5.12	-0.02	347267	54.0	35.9	25.9	48.1
					128.0	34.8	25.6	47.6




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.95	102.0	19.9	129.0	11.0







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.79	142.0	140.8	115.0	59.7











Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	113.1	115.0	67.8







Quantitation Results Report (QT Reviewed)







Quantitation Results Report (QT Reviewed)

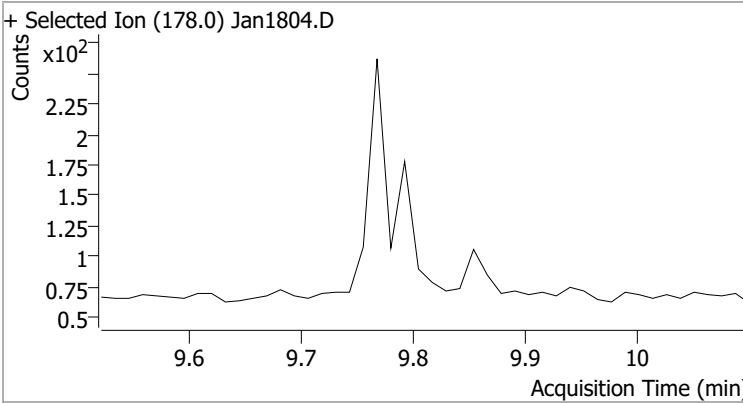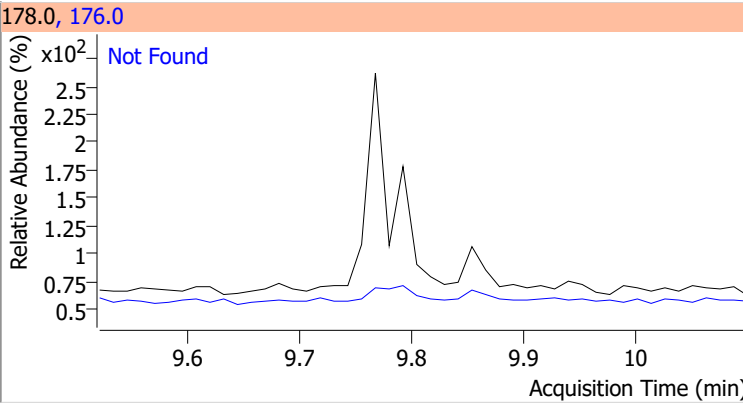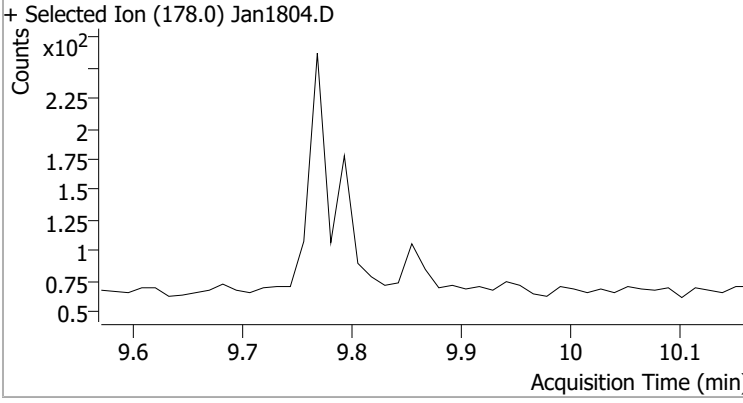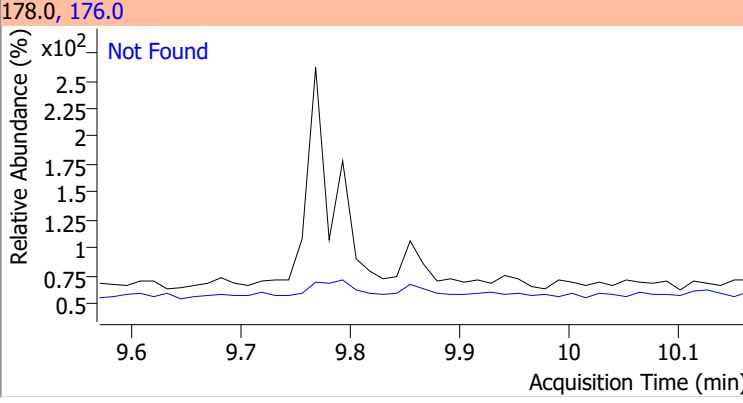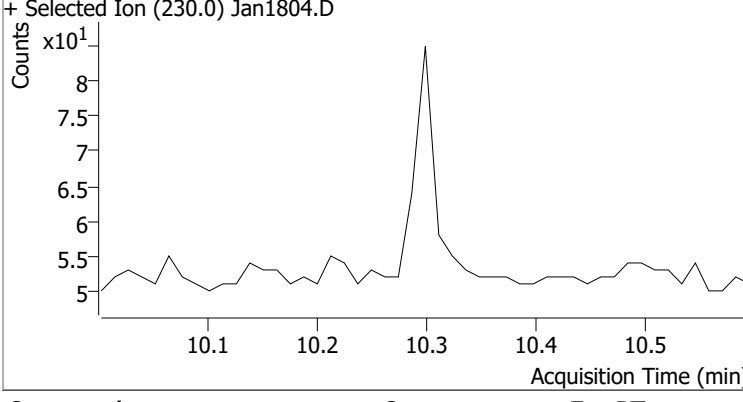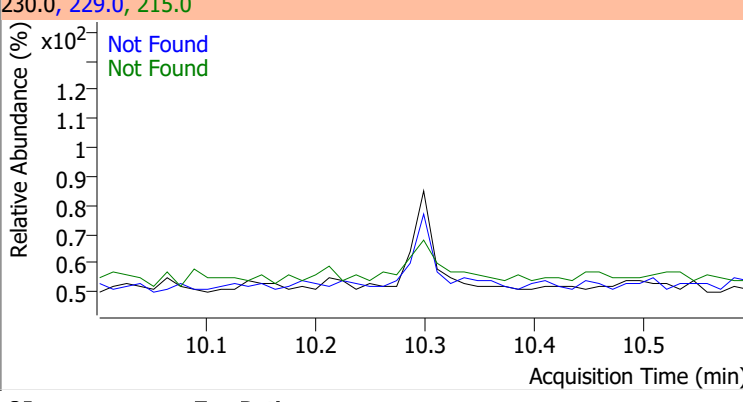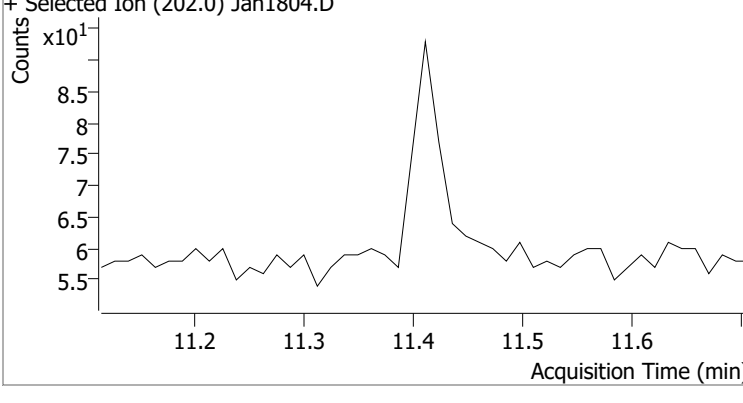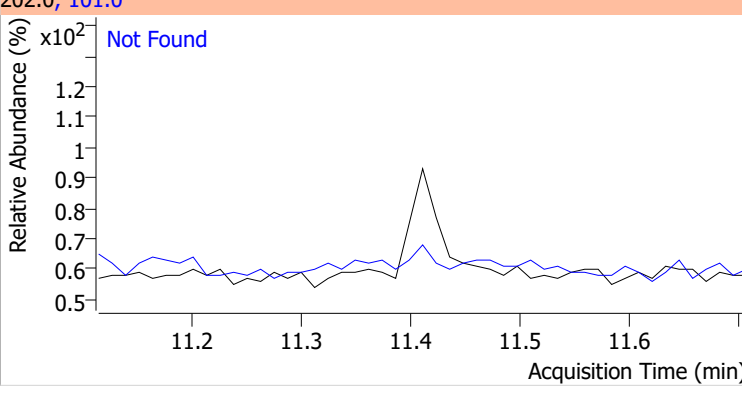Compound	Conc.	Exp RT	QIon	Exp Ratio		
Phenanthrene	N.D.	9.80	176.0	15.5		
+ Selected Ion (178.0) Jan1804.D 			178.0, 176.0 			
Anthracene	N.D.	9.87	176.0	18.1		
+ Selected Ion (178.0) Jan1804.D 			178.0, 176.0 			
o-Terphenyl	N.D.	10.30	229.0	70.2	QIon	Exp Ratio
			215.0	46.7		
+ Selected Ion (230.0) Jan1804.D 			230.0, 229.0, 215.0 			
Fluoranthene	N.D.	11.41	101.0	13.8		
+ Selected Ion (202.0) Jan1804.D 			202.0, 101.0 			

Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)

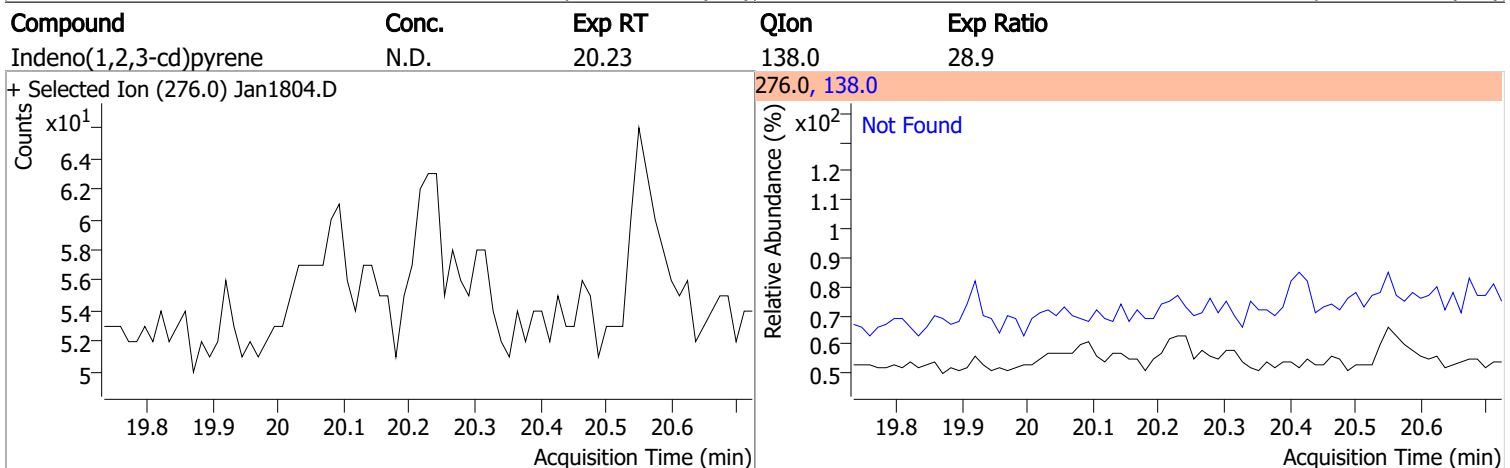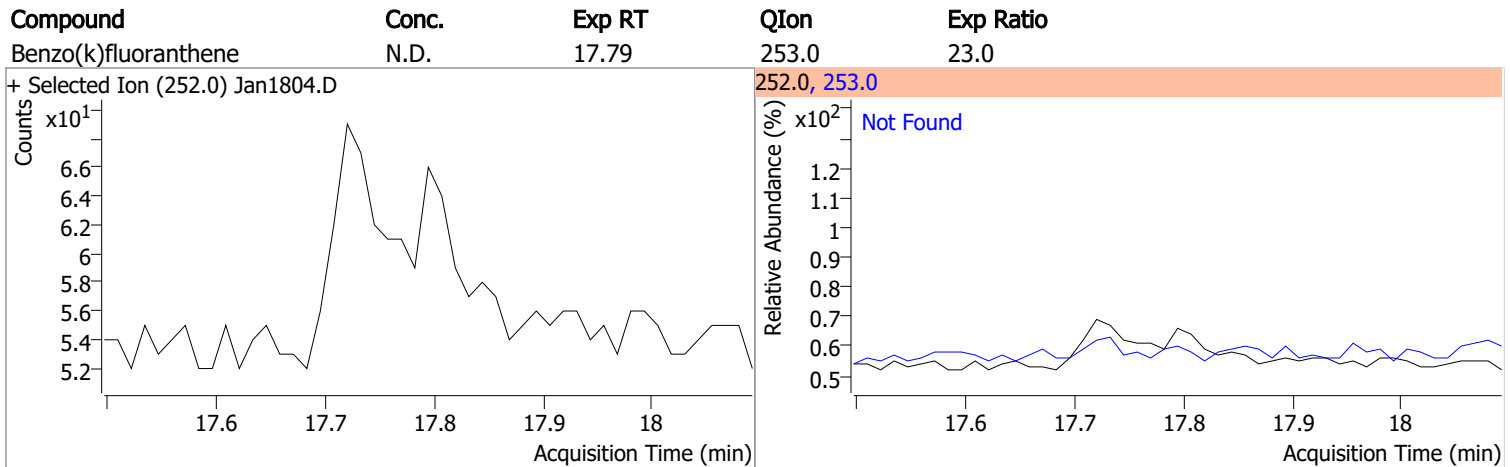


Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.30	279.0	25.1	139.0	24.1




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.56	138.0	28.0	277.0	23.3



Quantitation Results Report (QT Reviewed)

Data File	Jan1805.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/18/2022 5:32:39 PM
Sample Name	B22010211-001C	Instrument	GCMS
Vial	5	Multiplier	100.00
DA Method File	011722 bna SIM 1.batch.bin	Comment	SVOC-8270C-SIM-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011822 bna SIM1.batch.bin	Last Calib Update	1/17/2022 8:49:06 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
----------	----	------	-------	-------	-------	----------

Internal Standards

M 1,4-Dichlorobenzene-d4	4.484	152.0	184361	40.0000	ng/ml	-0.012
M Naphthalene-d8	5.928	136.0	330655	40.0000	ng/ml	-0.012
M Acenaphthene-d10	8.001	164.0	180725	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.768	188.0	353220	40.0000	ng/ml	-0.012
M Chrysene-d12	14.714	240.0	240323	40.0000	ng/ml	-0.012
M Perylene-d12	18.475	264.0	159643	40.0000	ng/ml	-0.025

System Monitoring Compounds

S Nitrobenzene-d5	5.143	82.0	0		ng/ml	md	0.000
Spiked Amount: 5.000		Range: 19.0 - 102.0%			Recovery = NA%		
S 2-Fluorobiphenyl	7.252	172.0	7859	90.4658	ng/ml		-0.012
Spiked Amount: 5.000		Range: 25.0 - 94.0%			Recovery = 1809.32% *		
S o-Terphenyl	0.000		0	N.D.			
Spiked Amount: 5.000		Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.251	244.0	5062	113.6197	ng/ml		-0.012
Spiked Amount: 5.000		Range: 39.0 - 106.0%			Recovery = 2272.39% *		

Target Compounds

Compound	RT	QIon	Resp.	Conc.	Units	#m	QValue
T Naphthalene	5.953	128.0	17159	150.0000	ng/ml	#m	67
T 2-Methylnaphthalene	6.777	141.0	54342	851.1025	ng/ml		72
T 1-Methylnaphthalene	6.890	141.0	39987	593.7996	ng/ml		95
T Acenaphthylene	7.839	152.0	0		ng/ml	md	1
T Acenaphthene	8.001	154.0	0		ng/ml	md	1
T Fluorene	8.661	166.0	0		ng/ml	md	1
T Phenanthrene	0.000		0	N.D.			
T Anthracene	0.000		0	N.D.			
T Fluoranthene	0.000		0	N.D.			
T Pyrene	0.000		0	N.D.			
T Benzo(a)Anthracene	14.702	228.0	0		ng/ml	md	1
T Chrysene	14.702	228.0	0		ng/ml	md	1
T Benzo(b)fluoranthene	0.000		0	N.D.			


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.376	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5		0		0	54.0 128.0		25.9 25.6	48.1 47.6



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	150.0000	5.95	0.00	17159 (m)	102.0 129.0	26.8 35.4	0.0 7.7	59.6 14.3




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	851.1025	6.78	-0.01	54342	142.0 115.0	100.3 70.5	98.5 41.8	183.0 77.6




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	593.7996	6.89	-0.01	39987	142.0	109.9	79.2	147.1
					115.0	60.6	47.5	88.2




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	90.4658	7.25	-0.01	7859	171.0	38.9	26.6	49.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthylene	0	0	0	0	153.0	-	9.0	16.6




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	0	0	0	0	153.0	-	82.1	152.6
					152.0	-	41.0	76.1




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene		0		0	165.0		69.1	128.3
					167.0		9.7	18.0




Compound	Conc.	Exp RT	QIon	Exp Ratio
Phenanthrene	N.D.	9.80	176.0	15.5







Compound	Conc.	Exp RT	QIon	Exp Ratio
Anthracene	N.D.	9.87	176.0	18.1



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
o-Terphenyl	N.D.	10.30	229.0	70.2	215.0	46.7




Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	0	0		0	226.0 229.0		21.2 15.0	39.4 27.8




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.73	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.79	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene	0	0		0	253.0		16.5	30.6




Quantitation Results Report (QT Reviewed)

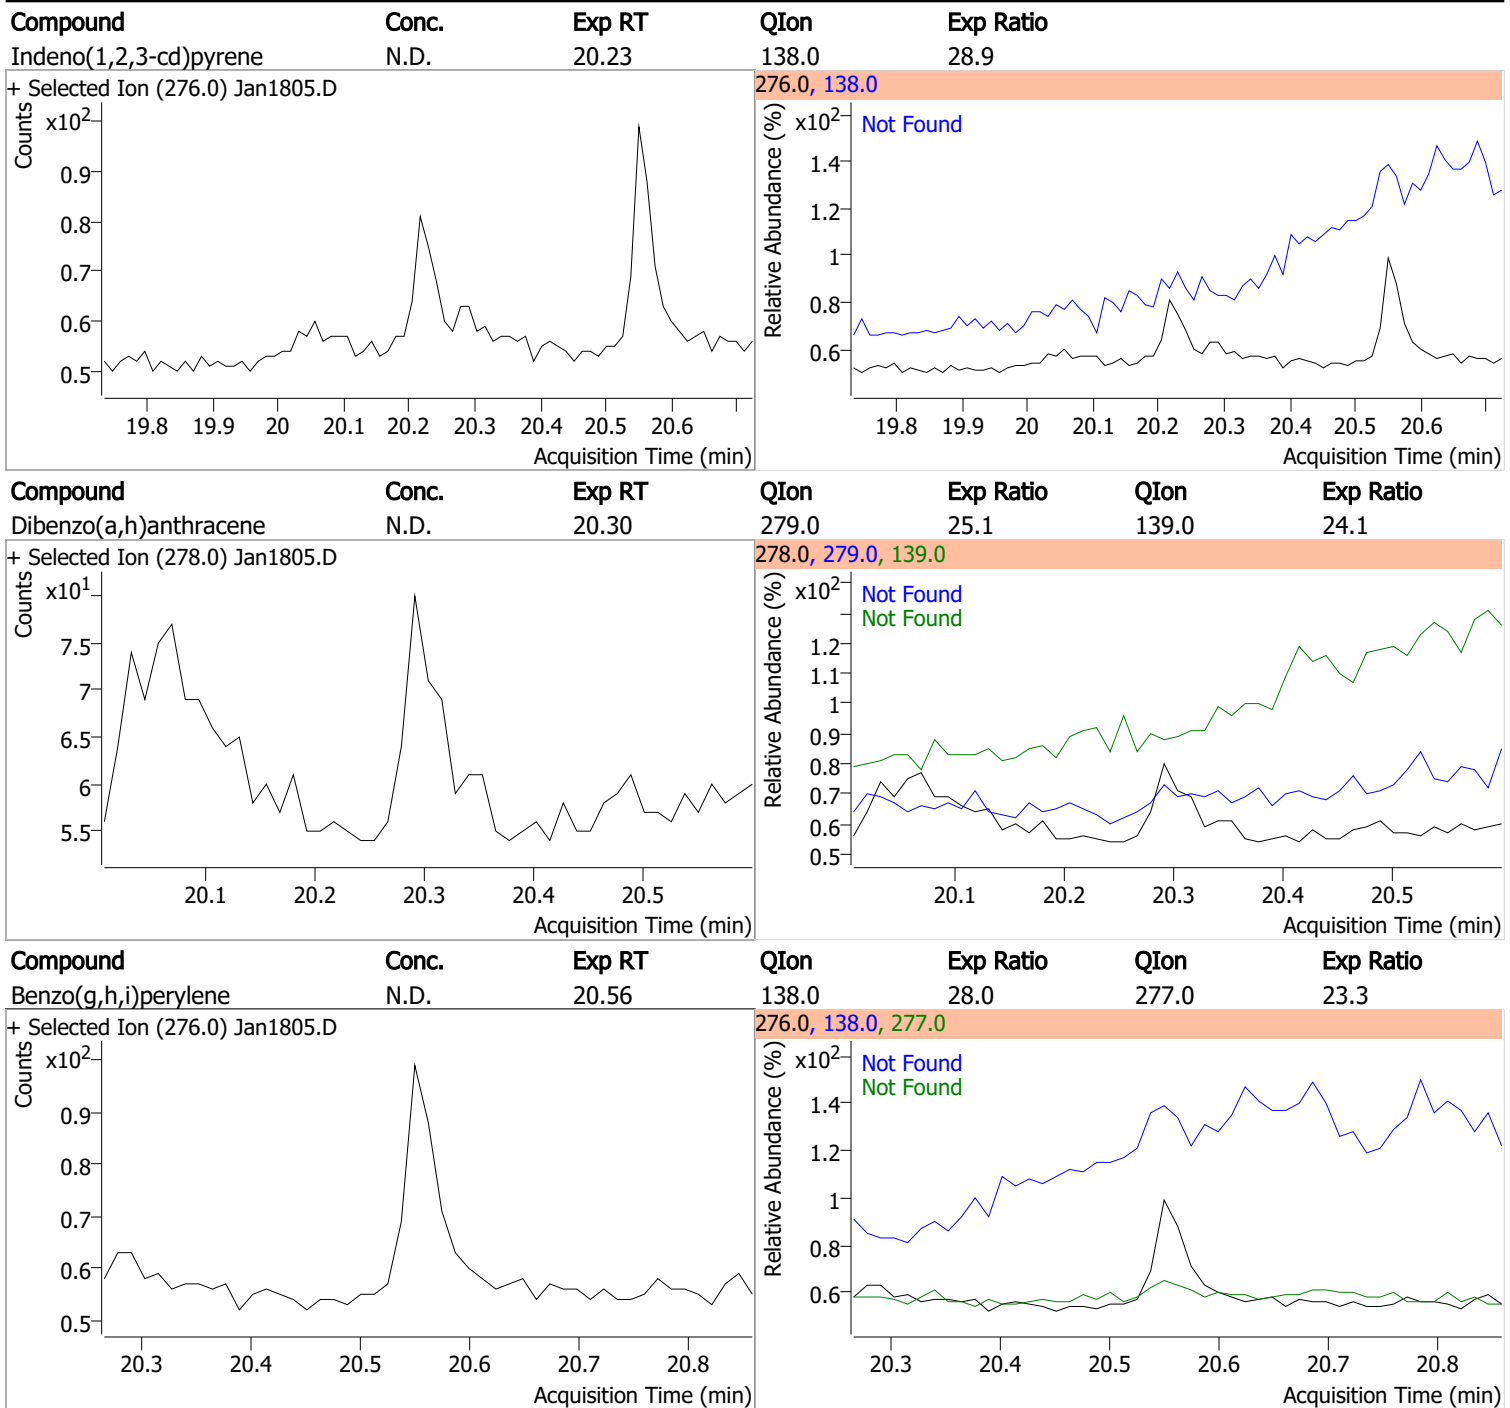

Quantitation Results Report (QT Reviewed)

Data File	Jan1806.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/18/2022 6:05:10 PM
Sample Name	LLCS-162800	Instrument	GCMS
Vial	6	Multiplier	20.00
DA Method File	011722 bna SIM 1.batch.bin	Comment	SVOC-8270C-SIM-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011822 bna SIM1.batch.bin	Last Calib Update	1/17/2022 8:49:06 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.484	152.0	176214	40.0000	ng/ml	-0.012
M Naphthalene-d8	5.928	136.0	314845	40.0000	ng/ml	-0.012
M Acenaphthene-d10	8.001	164.0	184782	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.768	188.0	348421	40.0000	ng/ml	-0.012
M Chrysene-d12	14.714	240.0	247599	40.0000	ng/ml	-0.012
M Perylene-d12	18.475	264.0	167071	40.0000	ng/ml	-0.025
System Monitoring Compounds						
S Nitrobenzene-d5	5.131	82.0	14583	78.5615	ng/ml	-0.012
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 1571.23%	*	
S 2-Fluorobiphenyl	7.252	172.0	33068	74.4628	ng/ml	-0.012
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1489.26%	*	
S o-Terphenyl	10.299	230.0	1361	4.8002	ng/ml	0.000
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = 96.00%		
S Terphenyl-d14	12.251	244.0	28037	121.1364	ng/ml	-0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 2422.73%	*	
Target Compounds						
T Naphthalene	5.953	128.0	1710	3.1404	ng/ml	# 1
T 2-Methylnaphthalene	6.790	141.0	987	3.2481	ng/ml	93
T 1-Methylnaphthalene	6.890	141.0	1080	3.3673	ng/ml	86
T Acenaphthylene	7.826	152.0	1869	3.3017	ng/ml	95
T Acenaphthene	8.038	154.0	1454	4.0132	ng/ml	m 95
T Fluorene	8.674	166.0	1795	4.1889	ng/ml	99
T Phenanthrene	9.793	178.0	3195	5.2752	ng/ml	93
T Anthracene	9.854	178.0	2636	5.1669	ng/ml	97
T Fluoranthene	11.411	202.0	3034	5.1349	ng/ml	97
T Pyrene	11.781	202.0	3293	5.2803	ng/ml	98
T Benzo(a)Anthracene	14.677	228.0	3292	5.9215	ng/ml	93
T Chrysene	14.776	228.0	3225	5.6911	ng/ml	96
T Benzo(b)fluoranthene	17.721	252.0	1930	5.1285	ng/ml	96


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	17.783	252.0	2070	4.6911	ng/ml	98
T Benzo(a)pyrene	18.363	252.0	1493	5.1108	ng/ml	95
T Indeno(1,2,3-cd)pyrene	20.217	276.0	1408	5.2616	ng/ml	97
T Dibenzo(a,h)anthracene	20.279	278.0	1735	5.1993	ng/ml	94
T Benzo(g,h,i)perylene	20.538	276.0	2063	4.9270	ng/ml	97


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	78.5615	5.13	-0.01	14583	54.0	35.0	25.9	48.1
					128.0	34.4	25.6	47.6



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	3.1404	5.95	0.00	1710	102.0	196.4	0.0	59.6
					129.0	15.5	7.7	14.3






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	3.2481	6.79	0.00	987	142.0	138.9	98.5	183.0
					115.0	43.8	41.8	77.6






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	3.3673	6.89	-0.01	1080	142.0	128.6	79.2	147.1
					115.0	57.7	47.5	88.2






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	74.4628	7.25	-0.01	33068	171.0	36.2	26.6	49.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthylene	3.3017	7.83	0.00	1869	153.0	14.9	9.0	16.6






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	4.0132	8.04	0.00	1454 (m)	153.0	110.5	82.1	152.6
					152.0	55.7	41.0	76.1






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene	4.1889	8.67	0.00	1795	165.0 167.0	99.6 14.4	69.1 9.7	128.3 18.0






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Phenanthrene	5.2752	9.79	-0.01	3195	176.0	18.4	10.8	20.1



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Anthracene	5.1669	9.85	-0.01	2636	176.0	19.3	12.7	23.5




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
o-Terphenyl	4.8002	10.30	0.00	1361	229.0 215.0	66.7 44.8	49.2 32.7	91.3 60.7




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluoranthene	5.1349	11.41	0.00	3034	101.0	12.7	9.6	17.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Pyrene	5.2803	11.78	-0.01	3293	101.0	16.2	10.7	20.0















Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	121.1364	12.25	-0.01	28037	122.0	19.9	13.4	25.0












Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)Anthracene	5.9215	14.68	-0.02	3292	226.0	23.7	18.9	35.1
					229.0	26.9	16.1	29.9



Quantitation Results Report (QT Reviewed)

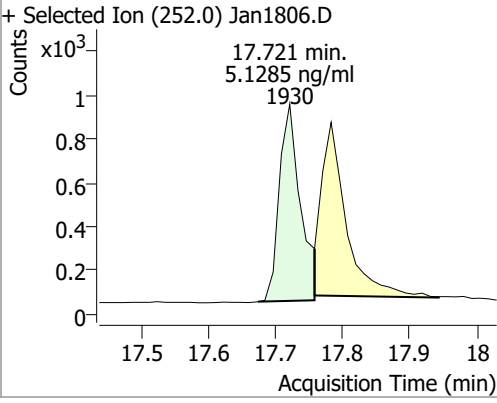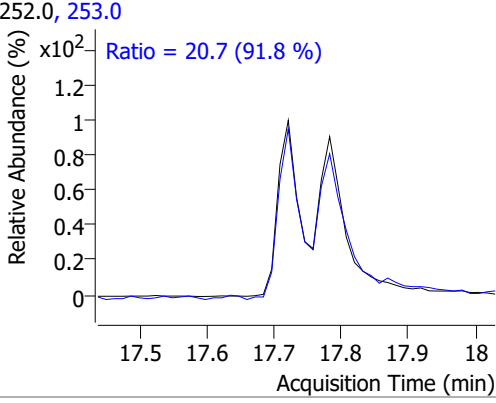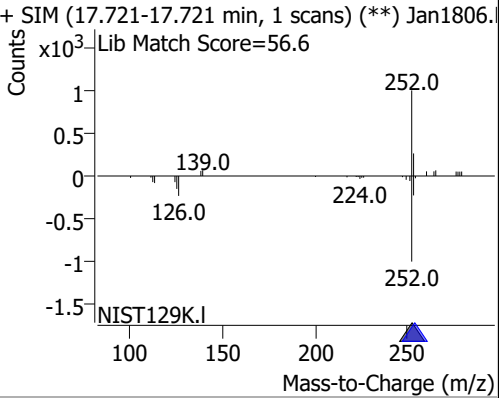Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	5.6911	14.78	-0.01	3225	226.0 229.0	32.2 19.5	21.2 15.0	39.4 27.8
+ Selected Ion (228.0) Jan1806.D 			228.0, 226.0, 229.0 			+ SIM (14.776-14.776 min, 1 scans) (**) Jan1806. Lib Match Score=43.3 		
Benzo(b)fluoranthene	5.1285	17.72	-0.01	1930	253.0	20.7	15.8	29.4
+ Selected Ion (252.0) Jan1806.D 			252.0, 253.0 			+ SIM (17.721-17.721 min, 1 scans) (**) Jan1806. Lib Match Score=56.6 		
Benzo(k)fluoranthene	4.6911	17.78	-0.01	2070	253.0	24.0	16.1	29.9
+ Selected Ion (252.0) Jan1806.D 			252.0, 253.0 			+ SIM (17.783-17.783 min, 1 scans) (**) Jan1806. Lib Match Score=56.0 		
Benzo(a)pyrene	5.1108	18.36	-0.01	1493	253.0	20.8	16.5	30.6
+ Selected Ion (252.0) Jan1806.D 			252.0, 253.0 			+ SIM (18.363-18.363 min, 1 scans) (**) Jan1806. Lib Match Score=54.7 		


Quantitation Results Report (QT Reviewed)

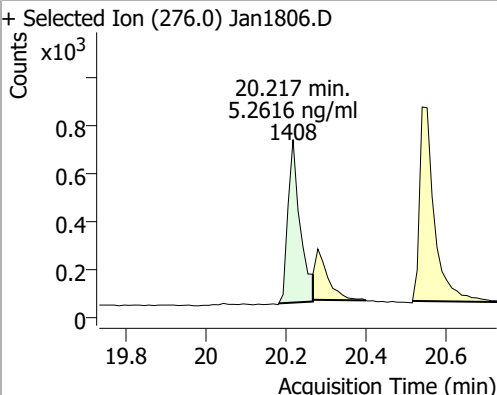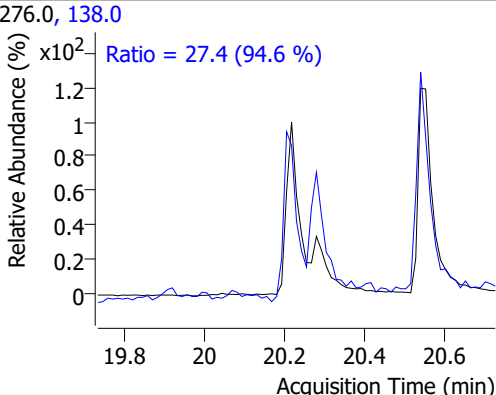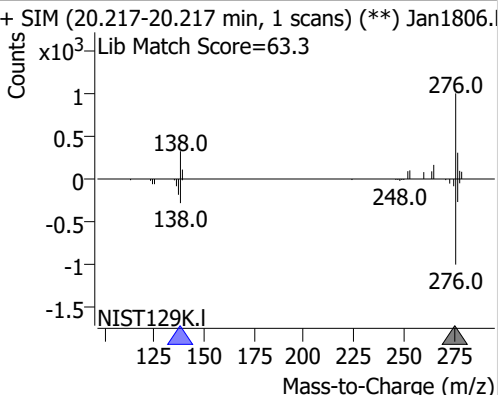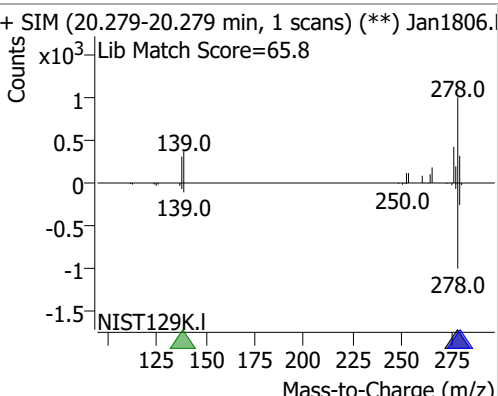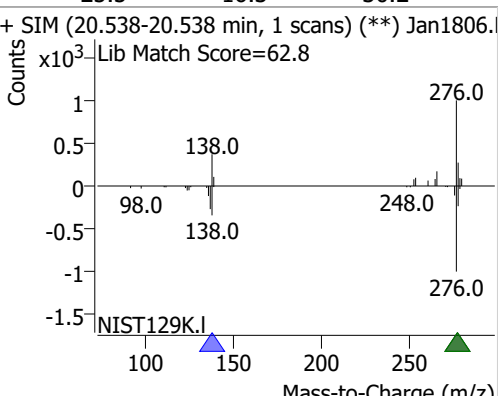Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Indeno(1,2,3-cd)pyrene	5.2616	20.22	-0.01	1408	138.0	27.4	20.3	37.6
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1806.D</p>  </div> <div style="width: 30%;"> <p>276.0, 138.0</p> <p>Ratio = 27.4 (94.6 %)</p>  </div> <div style="width: 30%;"> <p>+ SIM (20.217-20.217 min, 1 scans) (**) Jan1806.D</p> <p>Lib Match Score=63.3</p>  </div> </div>								
Dibenzo(a,h)anthracene	5.1993	20.28	-0.02	1735	279.0	20.7	17.6	32.7
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (278.0) Jan1806.D</p>  </div> <div style="width: 30%;"> <p>278.0, 279.0, 139.0</p> <p>Ratio = 20.7 (82.3 %)</p> <p>Ratio = 22.1 (91.9 %)</p>  </div> <div style="width: 30%;"> <p>+ SIM (20.279-20.279 min, 1 scans) (**) Jan1806.D</p> <p>Lib Match Score=65.8</p>  </div> </div>								
Benzo(g,h,i)perylene	4.9270	20.54	-0.02	2063	138.0	26.7	19.6	36.5
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1806.D</p>  </div> <div style="width: 30%;"> <p>276.0, 138.0, 277.0</p> <p>Ratio = 26.7 (95.3 %)</p> <p>Ratio = 25.5 (109.9 %)</p>  </div> <div style="width: 30%;"> <p>+ SIM (20.538-20.538 min, 1 scans) (**) Jan1806.D</p> <p>Lib Match Score=62.8</p>  </div> </div>								

Quantitation Results Report (QT Reviewed)

Data File	Jan1807.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/18/2022 6:37:25 PM
Sample Name	LLCSD-162800	Instrument	GCMS
Vial	7	Multiplier	1.00
DA Method File	011722 bna SIM 1.batch.bin	Comment	SVOC-8270C-SIM-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011822 bna SIM1.batch.bin	Last Calib Update	1/17/2022 8:49:06 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.484	152.0	173793	40.0000	ng/ml	-0.012
M Naphthalene-d8	5.928	136.0	328759	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.000	164.0	186798	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.768	188.0	367980	40.0000	ng/ml	-0.012
M Chrysene-d12	14.714	240.0	246570	40.0000	ng/ml	-0.012
M Perylene-d12	18.474	264.0	168105	40.0000	ng/ml	-0.025
System Monitoring Compounds						
S Nitrobenzene-d5	5.118	82.0	16460	4.3973	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 87.95%		
S 2-Fluorobiphenyl	7.252	172.0	29152	3.2468	ng/ml	-0.013
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 64.94%		
S o-Terphenyl	10.299	230.0	25981	4.3381	ng/ml	0.000
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = 86.76%		
S Terphenyl-d14	12.251	244.0	25395	5.5249	ng/ml	-0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 110.50%		*
Target Compounds						
T Naphthalene	5.941	128.0	30057	2.6426	ng/ml	98
T 2-Methylnaphthalene	6.777	141.0	19116	3.0111	ng/ml	89
T 1-Methylnaphthalene	6.890	141.0	17309	2.5851	ng/ml	96
T Acenaphthylene	7.826	152.0	35265	3.0805	ng/ml	98
T Acenaphthene	8.038	154.0	22319	3.0478	ng/ml	94
T Fluorene	8.661	166.0	31491	3.6343	ng/ml	100
T Phenanthrene	9.793	178.0	53464	4.6875	ng/ml	92
T Anthracene	9.854	178.0	49007	4.8068	ng/ml	99
T Fluoranthene	11.398	202.0	57952	4.6435	ng/ml	98
T Pyrene	11.781	202.0	61268	4.9324	ng/ml	99
T Benzo(a)Anthracene	14.677	228.0	42918	5.4141	ng/ml	99
T Chrysene	14.776	228.0	57173	5.0662	ng/ml	98
T Benzo(b)fluoranthene	17.708	252.0	40214	5.3097	ng/ml	98


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	17.770	252.0	44104	4.9786	ng/ml	96
T Benzo(a)pyrene	18.351	252.0	31577	5.0962	ng/ml	100
T Indeno(1,2,3-cd)pyrene	20.204	276.0	29416	4.9583	ng/ml	99
T Dibenzo(a,h)anthracene	20.278	278.0	34057	5.0714	ng/ml	98
T Benzo(g,h,i)perylene	20.538	276.0	42127	5.0085	ng/ml	98


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	4.3973	5.12	-0.02	16460	54.0	35.6	25.9	48.1
					128.0	34.1	25.6	47.6



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	2.6426	5.94	-0.01	30057	102.0	18.8	0.0	59.6
					129.0	10.8	7.7	14.3




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	3.0111	6.78	-0.01	19116	142.0	159.9	98.5	183.0
					115.0	58.7	41.8	77.6




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	2.5851	6.89	-0.01	17309	142.0	113.6	79.2	147.1
					115.0	59.5	47.5	88.2




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	3.2468	7.25	-0.01	29152	171.0	36.4	26.6	49.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthylene	3.0805	7.83	0.00	35265	153.0	12.2	9.0	16.6






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	3.0478	8.04	0.00	22319	153.0	109.4	82.1	152.6
					152.0	55.7	41.0	76.1






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene	3.6343	8.66	-0.01	31491	165.0	98.6	69.1	128.3
					167.0	13.3	9.7	18.0






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Phenanthrene	4.6875	9.79	-0.01	53464	176.0	19.0	10.8	20.1



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Anthracene	4.8068	9.85	-0.01	49007	176.0	18.6	12.7	23.5




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
o-Terphenyl	4.3381	10.30	0.00	25981	229.0	69.0	49.2	91.3
					215.0	45.3	32.7	60.7




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluoranthene	4.6435	11.40	-0.01	57952	101.0	13.1	9.6	17.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Pyrene	4.9324	11.78	-0.01	61268	101.0	15.9	10.7	20.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	5.5249	12.25	-0.01	25395	122.0	19.5	13.4	25.0




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)Anthracene	5.4141	14.68	-0.02	42918	226.0	27.5	18.9	35.1
					229.0	22.4	16.1	29.9




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	5.0662	14.78	-0.01	57173	226.0	30.1	21.2	39.4
					229.0	19.5	15.0	27.8




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(b)fluoranthene	5.3097	17.71	-0.02	40214	253.0	21.8	15.8	29.4



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(k)fluoranthene	4.9786	17.77	-0.02	44104	253.0	21.3	16.1	29.9



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene	5.0962	18.35	-0.02	31577	253.0	23.6	16.5	30.6




Quantitation Results Report (QT Reviewed)

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Indeno(1,2,3-cd)pyrene	4.9583	20.20	-0.02	29416	138.0	28.5	20.3	37.6
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1807.D</p> </div> <div style="width: 30%;"> <p>276.0, 138.0</p> <p>Ratio = 28.5 (98.7 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.204-20.204 min, 1 scans) (**) Jan1807.D</p> <p>Lib Match Score=78.5</p> </div> </div>								
Dibenzo(a,h)anthracene	5.0714	20.28	-0.02	34057	279.0	25.0	17.6	32.7
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (278.0) Jan1807.D</p> </div> <div style="width: 30%;"> <p>278.0, 279.0, 139.0</p> <p>Ratio = 25.0 (99.5 %)</p> <p>Ratio = 22.6 (94.0 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.278-20.278 min, 1 scans) (**) Jan1807.D</p> <p>Lib Match Score=77.7</p> </div> </div>								
Benzo(g,h,i)perylene	5.0085	20.54	-0.02	42127	138.0	27.0	19.6	36.5
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1807.D</p> </div> <div style="width: 30%;"> <p>276.0, 138.0, 277.0</p> <p>Ratio = 27.0 (96.3 %)</p> <p>Ratio = 23.9 (103.0 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.538-20.538 min, 1 scans) (**) Jan1807.D</p> <p>Lib Match Score=78.3</p> </div> </div>								

Quantitation Results Report (QT Reviewed)

Data File	Jan1808.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/18/2022 7:09:45 PM
Sample Name	LLCS-162889	Instrument	GCMS
Vial	8	Multiplier	1.00
DA Method File	011722 bna SIM 1.batch.bin	Comment	SVOC-8270C-SIM-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011822 bna SIM1.batch.bin	Last Calib Update	1/17/2022 8:49:06 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.484	152.0	183763	40.0000	ng/ml	-0.012
M Naphthalene-d8	5.928	136.0	340311	40.0000	ng/ml	-0.012
M Acenaphthene-d10	8.000	164.0	200371	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.768	188.0	390696	40.0000	ng/ml	-0.012
M Chrysene-d12	14.714	240.0	271804	40.0000	ng/ml	-0.012
M Perylene-d12	18.475	264.0	186246	40.0000	ng/ml	-0.025
System Monitoring Compounds						
S Nitrobenzene-d5	5.118	82.0	15832	4.0631	ng/ml	-0.025
Spiked Amount: 5.000		Range: 19.0 - 102.0%		Recovery = 81.26%		
S 2-Fluorobiphenyl	7.252	172.0	32670	3.3921	ng/ml	-0.012
Spiked Amount: 5.000		Range: 25.0 - 94.0%		Recovery = 67.84%		
S o-Terphenyl	10.299	230.0	26559	4.1768	ng/ml	0.000
Spiked Amount: 5.000		Range: 40.0 - 140.0%		Recovery = 83.54%		
S Terphenyl-d14	12.251	244.0	25537	5.0528	ng/ml	-0.012
Spiked Amount: 5.000		Range: 39.0 - 106.0%		Recovery = 101.06%		
Target Compounds						
T Naphthalene	5.941	128.0	34410	2.9227	ng/ml	98
T 2-Methylnaphthalene	6.777	141.0	23065	3.5099	ng/ml	93
T 1-Methylnaphthalene	6.890	141.0	20412	2.9451	ng/ml	96
T Acenaphthylene	7.826	152.0	39670	3.2306	ng/ml	100
T Acenaphthene	8.038	154.0	26296	3.3477	ng/ml	94
T Fluorene	8.661	166.0	36028	3.8763	ng/ml	99
T Phenanthrene	9.793	178.0	55579	4.5914	ng/ml	91
T Anthracene	9.854	178.0	50279	4.6531	ng/ml	98
T Fluoranthene	11.398	202.0	59346	4.4788	ng/ml	99
T Pyrene	11.781	202.0	61145	4.4655	ng/ml	97
T Benzo(a)Anthracene	14.677	228.0	43728	5.0260	ng/ml	99
T Chrysene	14.776	228.0	58387	4.6934	ng/ml	99
T Benzo(b)fluoranthene	17.708	252.0	41186	4.9083	ng/ml	99


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	17.770	252.0	42889	4.3921	ng/ml	99
T Benzo(a)pyrene	18.351	252.0	32467	4.7667	ng/ml	100
T Indeno(1,2,3-cd)pyrene	20.204	276.0	29317	4.5109	ng/ml	99
T Dibenzo(a,h)anthracene	20.278	278.0	34893	4.6898	ng/ml	98
T Benzo(g,h,i)perylene	20.538	276.0	43357	4.6795	ng/ml m	99


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	4.0631	5.12	-0.02	15832	54.0	35.7	25.9	48.1
					128.0	27.9	25.6	47.6



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	2.9227	5.94	-0.01	34410	102.0	18.5	0.0	59.6
					129.0	10.6	7.7	14.3




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	3.5099	6.78	-0.01	23065	142.0	150.4	98.5	183.0
					115.0	57.0	41.8	77.6




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	2.9451	6.89	-0.01	20412	142.0	116.1	79.2	147.1
					115.0	62.6	47.5	88.2




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	3.3921	7.25	-0.01	32670	171.0	35.8	26.6	49.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthylene	3.2306	7.83	0.00	39670	153.0	12.6	9.0	16.6






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	3.3477	8.04	0.00	26296	153.0	110.0	82.1	152.6
					152.0	55.3	41.0	76.1






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene	3.8763	8.66	-0.01	36028	165.0	97.7	69.1	128.3
					167.0	13.5	9.7	18.0






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Phenanthrene	4.5914	9.79	-0.01	55579	176.0	19.3	10.8	20.1
					178.0	19.3	125.0	19.3



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Anthracene	4.6531	9.85	-0.01	50279	176.0	18.8	12.7	23.5
					178.0	18.8	103.9	18.8




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
o-Terphenyl	4.1768	10.30	0.00	26559	229.0	69.1	49.2	91.3
					215.0	45.5	32.7	60.7
					230.0	69.1	98.4	69.1




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluoranthene	4.4788	11.40	-0.01	59346	101.0	13.2	9.6	17.9




Pyrene	4.4655	11.78	-0.01	61145	101.0	16.5	10.7	20.0
--------	--------	-------	-------	-------	-------	------	------	------



Terphenyl-d14	5.0528	12.25	-0.01	25537	122.0	19.8	13.4	25.0
---------------	--------	-------	-------	-------	-------	------	------	------




Benzo(a)Anthracene	5.0260	14.68	-0.02	43728	226.0 229.0	27.3 22.7	18.9 16.1	35.1 29.9
--------------------	--------	-------	-------	-------	----------------	--------------	--------------	--------------




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	4.6934	14.78	-0.01	58387	226.0	30.2	21.2	39.4
					229.0	20.5	15.0	27.8




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(b)fluoranthene	4.9083	17.71	-0.02	41186	253.0	22.0	15.8	29.4



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(k)fluoranthene	4.3921	17.77	-0.02	42889	253.0	23.6	16.1	29.9



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene	4.7667	18.35	-0.02	32467	253.0	23.6	16.5	30.6




Quantitation Results Report (QT Reviewed)

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Indeno(1,2,3-cd)pyrene	4.5109	20.20	-0.02	29317	138.0	29.4	20.3	37.6
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1808.D</p> </div> <div style="width: 30%;"> <p>276.0, 138.0</p> <p>Ratio = 29.4 (101.5 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.204-20.204 min, 1 scans) (**) Jan1808.D</p> <p>Lib Match Score=78.5</p> </div> </div>								
Dibenzo(a,h)anthracene	4.6898	20.28	-0.02	34893	279.0	24.5	17.6	32.7
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (278.0) Jan1808.D</p> </div> <div style="width: 30%;"> <p>278.0, 279.0, 139.0</p> <p>Ratio = 24.5 (97.6 %)</p> <p>Ratio = 22.5 (93.4 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.278-20.278 min, 1 scans) (**) Jan1808.D</p> <p>Lib Match Score=77.7</p> </div> </div>								
Benzo(g,h,i)perylene	4.6795	20.54	-0.02	43357 (m)	138.0	27.5	19.6	36.5
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1808.D</p> </div> <div style="width: 30%;"> <p>276.0, 138.0, 277.0</p> <p>Ratio = 27.5 (98.2 %)</p> <p>Ratio = 24.1 (103.5 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.538-20.538 min, 1 scans) (**) Jan1808.D</p> <p>Lib Match Score=78.4</p> </div> </div>								

Quantitation Results Report (QT Reviewed)

Data File	Jan1809.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/18/2022 7:42:02 PM
Sample Name	LLCSD-162889	Instrument	GCMS
Vial	9	Multiplier	1.00
DA Method File	011722 bna SIM 1.batch.bin	Comment	SVOC-8270C-SIM-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011822 bna SIM1.batch.bin	Last Calib Update	1/17/2022 8:49:06 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.484	152.0	180580	40.0000	ng/ml	-0.012
M Naphthalene-d8	5.928	136.0	328165	40.0000	ng/ml	-0.012
M Acenaphthene-d10	8.001	164.0	193647	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.768	188.0	389420	40.0000	ng/ml	-0.012
M Chrysene-d12	14.714	240.0	262106	40.0000	ng/ml	-0.012
M Perylene-d12	18.475	264.0	177129	40.0000	ng/ml	-0.025
System Monitoring Compounds						
S Nitrobenzene-d5	5.118	82.0	14710	3.8761	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%		Recovery = 77.52%			
S 2-Fluorobiphenyl	7.252	172.0	28496	3.0615	ng/ml	-0.012
Spiked Amount: 5.000	Range: 25.0 - 94.0%		Recovery = 61.23%			
S o-Terphenyl	10.299	230.0	25456	4.0164	ng/ml	0.000
Spiked Amount: 5.000	Range: 40.0 - 140.0%		Recovery = 80.33%			
S Terphenyl-d14	12.251	244.0	24746	5.0768	ng/ml	-0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%		Recovery = 101.54%			
Target Compounds						
T Naphthalene	5.941	128.0	27466	2.4192	ng/ml	99
T 2-Methylnaphthalene	6.777	141.0	17285	2.7277	ng/ml	89
T 1-Methylnaphthalene	6.890	141.0	15821	2.3672	ng/ml	96
T Acenaphthylene	7.826	152.0	33397	2.8142	ng/ml	99
T Acenaphthene	8.038	154.0	21251	2.7994	ng/ml	94
T Fluorene	8.661	166.0	31168	3.4698	ng/ml	100
T Phenanthrene	9.793	178.0	52360	4.3439	ng/ml	91
T Anthracene	9.854	178.0	48752	4.5328	ng/ml	99
T Fluoranthene	11.398	202.0	58358	4.4186	ng/ml	98
T Pyrene	11.781	202.0	59941	4.5396	ng/ml	97
T Benzo(a)Anthracene	14.677	228.0	43111	5.1325	ng/ml	99
T Chrysene	14.776	228.0	57291	4.7758	ng/ml	99
T Benzo(b)fluoranthene	17.709	252.0	40831	5.1165	ng/ml	99


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	17.770	252.0	44077	4.7322	ng/ml	99
T Benzo(a)pyrene	18.351	252.0	32014	4.9237	ng/ml	100
T Indeno(1,2,3-cd)pyrene	20.204	276.0	30029	4.8205	ng/ml	97
T Dibenzo(a,h)anthracene	20.266	278.0	35323	4.9919	ng/ml	96
T Benzo(g,h,i)perylene	20.538	276.0	42115	4.7717	ng/ml	98


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	3.8761	5.12	-0.02	14710	54.0	35.9	25.9	48.1
					128.0	28.5	25.6	47.6



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	2.4192	5.94	-0.01	27466	102.0	19.4	0.0	59.6
					129.0	10.7	7.7	14.3




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	2.7277	6.78	-0.01	17285	142.0	157.9	98.5	183.0
					115.0	56.0	41.8	77.6




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	2.3672	6.89	-0.01	15821	142.0	114.4	79.2	147.1
					115.0	60.9	47.5	88.2




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	3.0615	7.25	-0.01	28496	171.0	35.8	26.6	49.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthylene	2.8142	7.83	0.00	33397	153.0	12.3	9.0	16.6






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	2.7994	8.04	0.00	21251	153.0	110.0	82.1	152.6
					152.0	55.7	41.0	76.1






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene	3.4698	8.66	-0.01	31168	165.0	98.2	69.1	128.3
					167.0	13.6	9.7	18.0






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Phenanthrene	4.3439	9.79	-0.01	52360	176.0	19.2	10.8	20.1



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Anthracene	4.5328	9.85	-0.01	48752	176.0	18.7	12.7	23.5




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
o-Terphenyl	4.0164	10.30	0.00	25456	229.0	70.5	49.2	91.3
					215.0	46.8	32.7	60.7




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluoranthene	4.4186	11.40	-0.01	58358	101.0	13.0	9.6	17.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Pyrene	4.5396	11.78	-0.01	59941	101.0	16.4	10.7	20.0















Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	5.0768	12.25	-0.01	24746	122.0	19.4	13.4	25.0












Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)Anthracene	5.1325	14.68	-0.02	43111	226.0	27.4	18.9	35.1
					229.0	22.6	16.1	29.9



Quantitation Results Report (QT Reviewed)

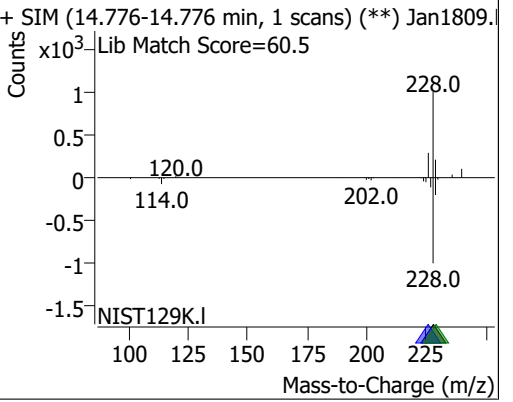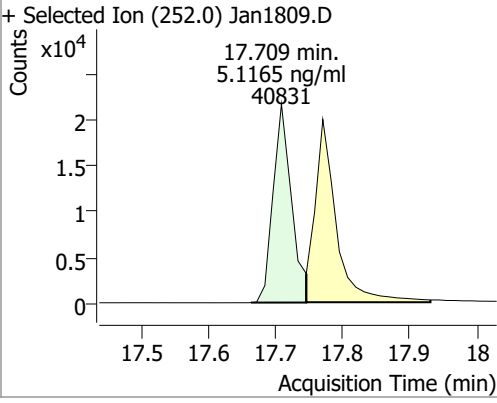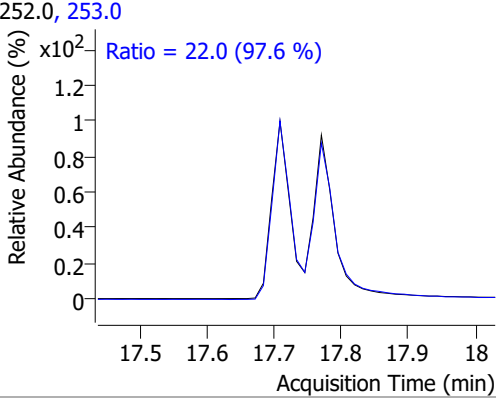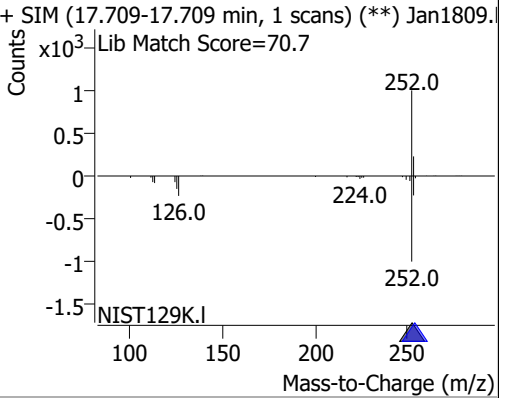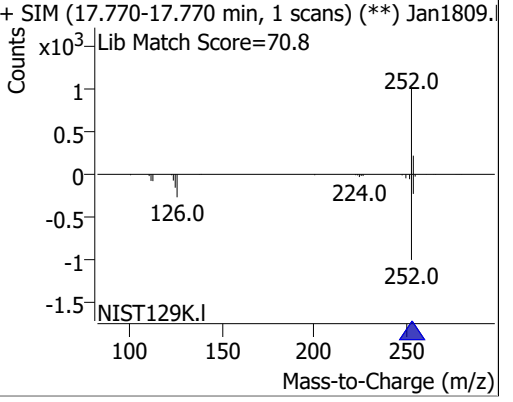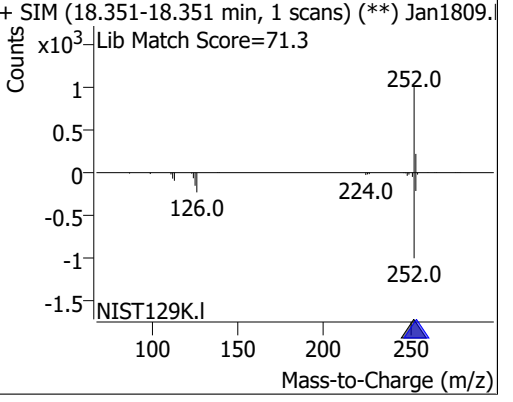Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	4.7758	14.78	-0.01	57291	226.0 229.0	30.1 20.8	21.2 15.0	39.4 27.8
+ Selected Ion (228.0) Jan1809.D 			228.0, 226.0, 229.0 			+ SIM (14.776-14.776 min, 1 scans) (**) Jan1809.D Lib Match Score=60.5 		
Benzo(b)fluoranthene	5.1165	17.71	-0.02	40831	253.0	22.0	15.8	29.4
+ Selected Ion (252.0) Jan1809.D 			252.0, 253.0 			+ SIM (17.709-17.709 min, 1 scans) (**) Jan1809.D Lib Match Score=70.7 		
Benzo(k)fluoranthene	4.7322	17.77	-0.02	44077	253.0	22.5	16.1	29.9
+ Selected Ion (252.0) Jan1809.D 			252.0, 253.0 			+ SIM (17.770-17.770 min, 1 scans) (**) Jan1809.D Lib Match Score=70.8 		
Benzo(a)pyrene	4.9237	18.35	-0.02	32014	253.0	23.7	16.5	30.6
+ Selected Ion (252.0) Jan1809.D 			252.0, 253.0 			+ SIM (18.351-18.351 min, 1 scans) (**) Jan1809.D Lib Match Score=71.3 		


Quantitation Results Report (QT Reviewed)

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Indeno(1,2,3-cd)pyrene	4.8205	20.20	-0.02	30029	138.0	27.5	20.3	37.6
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1809.D</p>  </div> <div style="width: 30%;"> <p>276.0, 138.0</p> <p>Ratio = 27.5 (95.0 %)</p>  </div> <div style="width: 30%;"> <p>+ SIM (20.204-20.204 min, 1 scans) (**) Jan1809.D</p> <p>Lib Match Score=78.5</p>  </div> </div>								
Dibenzo(a,h)anthracene	4.9919	20.27	-0.04	35323	279.0	23.8	17.6	32.7
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (278.0) Jan1809.D</p>  </div> <div style="width: 30%;"> <p>278.0, 279.0, 139.0</p> <p>Ratio = 23.8 (94.8 %)</p> <p>Ratio = 21.3 (88.5 %)</p>  </div> <div style="width: 30%;"> <p>+ SIM (20.266-20.266 min, 1 scans) (**) Jan1809.D</p> <p>Lib Match Score=75.8</p>  </div> </div>								
Benzo(g,h,i)perylene	4.7717	20.54	-0.02	42115	138.0	27.1	19.6	36.5
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1809.D</p>  </div> <div style="width: 30%;"> <p>276.0, 138.0, 277.0</p> <p>Ratio = 27.1 (96.5 %)</p> <p>Ratio = 24.1 (103.9 %)</p>  </div> <div style="width: 30%;"> <p>+ SIM (20.538-20.538 min, 1 scans) (**) Jan1809.D</p> <p>Lib Match Score=78.6</p>  </div> </div>								

Quantitation Results Report (QT Reviewed)

Data File	Jan1810.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/18/2022 8:14:24 PM
Sample Name	MB-162889	Instrument	GCMS
Vial	10	Multiplier	1.00
DA Method File	011722 bna SIM 1.batch.bin	Comment	SVOC-8270C-SIM-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011822 bna SIM1.batch.bin	Last Calib Update	1/17/2022 8:49:06 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.485	152.0	180993	40.0000	ng/ml	-0.012
M Naphthalene-d8	5.928	136.0	320475	40.0000	ng/ml	-0.012
M Acenaphthene-d10	8.001	164.0	181027	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.768	188.0	358385	40.0000	ng/ml	-0.012
M Chrysene-d12	14.702	240.0	242638	40.0000	ng/ml	-0.025
M Perylene-d12	18.475	264.0	156939	40.0000	ng/ml	-0.024
System Monitoring Compounds						
S Nitrobenzene-d5	5.118	82.0	340128	35.6956	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 713.91%		*
S 2-Fluorobiphenyl	7.252	172.0	540891	62.1615	ng/ml	-0.012
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1243.23%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.251	244.0	512732	77.5887	ng/ml	-0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 1551.77%		*
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.001	154.0	0		ng/ml	md 1
T Fluorene	8.960	166.0	0		ng/ml	md 1
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.702	228.0	0		ng/ml	md 1
T Chrysene	14.776	228.0	0		ng/ml	md 1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.364	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	35.6956	5.12	-0.02	340128	54.0	35.9	25.9	48.1
					128.0	34.8	25.6	47.6




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.95	102.0	19.9	129.0	11.0







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.79	142.0	140.8	115.0	59.7







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	113.1	115.0	67.8







Quantitation Results Report (QT Reviewed)

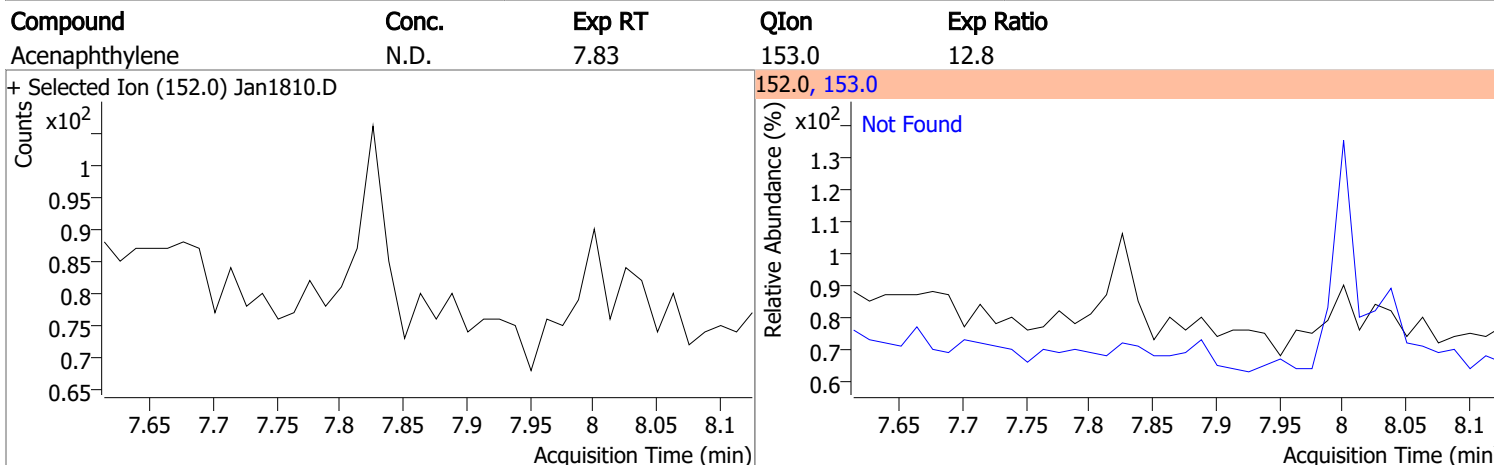

Quantitation Results Report (QT Reviewed)

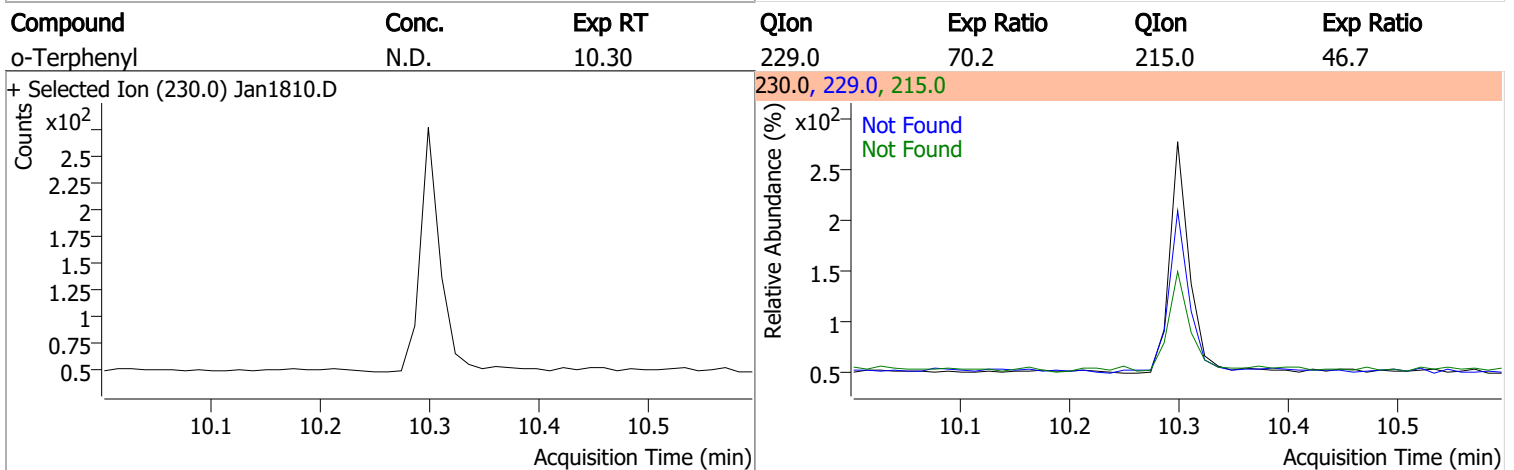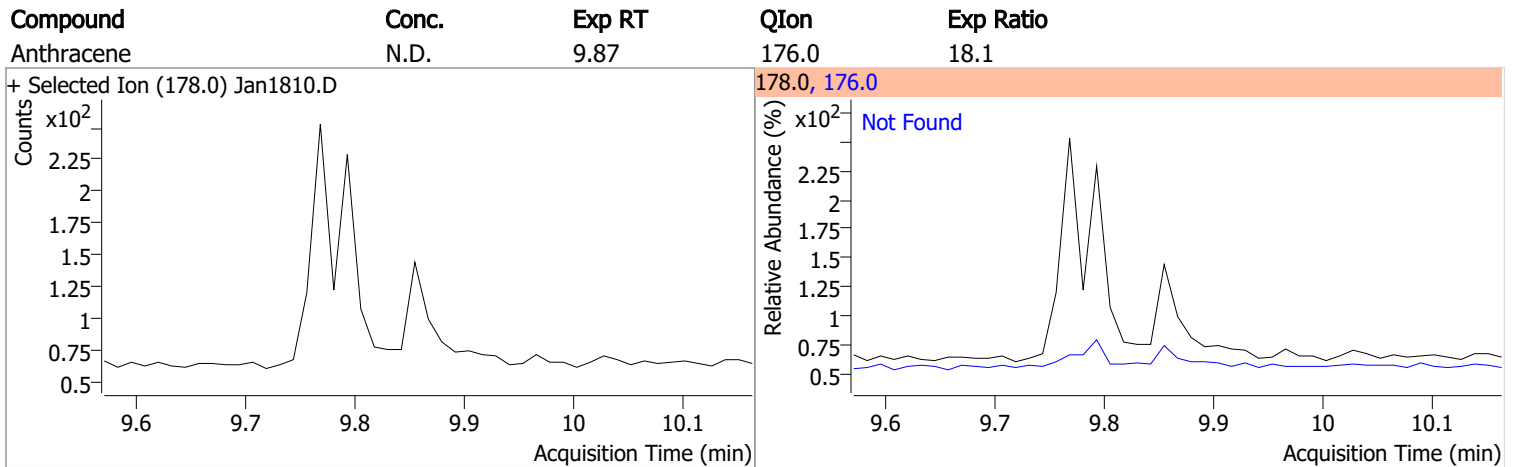


Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.73	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.79	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.5	30.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.23	138.0	28.9




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.30	279.0	25.1	139.0	24.1




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.56	138.0	28.0	277.0	23.3



Quantitation Results Report (QT Reviewed)

Data File	Jan1811.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/18/2022 8:46:41 PM
Sample Name	B22010507-001C	Instrument	GCMS
Vial	11	Multiplier	1.00
DA Method File	011722 bna SIM 1.batch.bin	Comment	SVOC-8270C-SIM-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011822 bna SIM1.batch.bin	Last Calib Update	1/17/2022 8:49:06 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.484	152.0	194230	40.0000	ng/ml	-0.012
M Naphthalene-d8	5.928	136.0	337427	40.0000	ng/ml	-0.012
M Acenaphthene-d10	8.000	164.0	193221	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.768	188.0	388035	40.0000	ng/ml	-0.012
M Chrysene-d12	14.714	240.0	258971	40.0000	ng/ml	-0.012
M Perylene-d12	18.475	264.0	174431	40.0000	ng/ml	-0.025
System Monitoring Compounds						
S Nitrobenzene-d5	5.118	82.0	351252	34.8846	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 697.69%		*
S 2-Fluorobiphenyl	7.252	172.0	536422	57.7573	ng/ml	-0.012
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1155.15%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.251	244.0	539297	76.7475	ng/ml	-0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 1534.95%		*
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.000	154.0	0		ng/ml	md
T Fluorene	8.960	166.0	0		ng/ml	md
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.701	228.0	0		ng/ml	md
T Chrysene	14.776	228.0	0		ng/ml	md
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.475	252.0	0		ng/ml md	1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	34.8846	5.12	-0.02	351252	54.0	35.5	25.9	48.1
					128.0	33.5	25.6	47.6




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.95	102.0	19.9	129.0	11.0







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.79	142.0	140.8	115.0	59.7



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	113.1	115.0	67.8







Quantitation Results Report (QT Reviewed)



Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio	
Phenanthrene	N.D.	9.80	176.0	15.5	
+ Selected Ion (178.0) Jan1811.D			178.0, 176.0		
Anthracene	N.D.	9.87	176.0	18.1	
+ Selected Ion (178.0) Jan1811.D			178.0, 176.0		
o-Terphenyl	N.D.	10.30	229.0	70.2	QIon: 215.0, Exp Ratio: 46.7
+ Selected Ion (230.0) Jan1811.D			230.0, 229.0, 215.0		
Fluoranthene	N.D.	11.41	101.0	13.8	
+ Selected Ion (202.0) Jan1811.D			202.0, 101.0		

Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.73	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.79	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.5	30.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.23	138.0	28.9




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.30	279.0	25.1	139.0	24.1




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.56	138.0	28.0	277.0	23.3



Quantitation Results Report (QT Reviewed)

Data File	Jan1812.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/18/2022 9:19:01 PM
Sample Name	B22010625-001C	Instrument	GCMS
Vial	12	Multiplier	1.00
DA Method File	011722 bna SIM 1.batch.bin	Comment	SVOC-8270C-SIM-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011822 bna SIM1.batch.bin	Last Calib Update	1/17/2022 8:49:06 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.484	152.0	175278	40.0000	ng/ml	-0.012
M Naphthalene-d8	5.928	136.0	308221	40.0000	ng/ml	-0.012
M Acenaphthene-d10	8.001	164.0	182428	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.768	188.0	345870	40.0000	ng/ml	-0.012
M Chrysene-d12	14.702	240.0	247260	40.0000	ng/ml	-0.025
M Perylene-d12	18.475	264.0	161590	40.0000	ng/ml	-0.025
System Monitoring Compounds						
S Nitrobenzene-d5	5.118	82.0	327251	35.5570	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 711.14%		*
S 2-Fluorobiphenyl	7.252	172.0	557143	63.5376	ng/ml	-0.012
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1270.75%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.251	244.0	485777	73.4739	ng/ml	-0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 1469.48%		*
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.025	154.0	0		ng/ml	md
T Fluorene	8.960	166.0	0		ng/ml	md
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.702	228.0	0		ng/ml	md
T Chrysene	14.702	228.0	0		ng/ml	md
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.475	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	35.5570	5.12	-0.02	327251	54.0	34.7	25.9	48.1
					128.0	32.8	25.6	47.6




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.95	102.0	19.9	129.0	11.0







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.79	142.0	140.8	115.0	59.7











Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	113.1	115.0	67.8







Quantitation Results Report (QT Reviewed)



Quantitation Results Report (QT Reviewed)

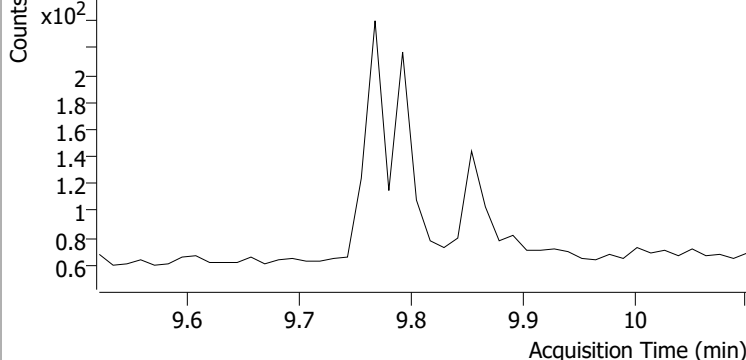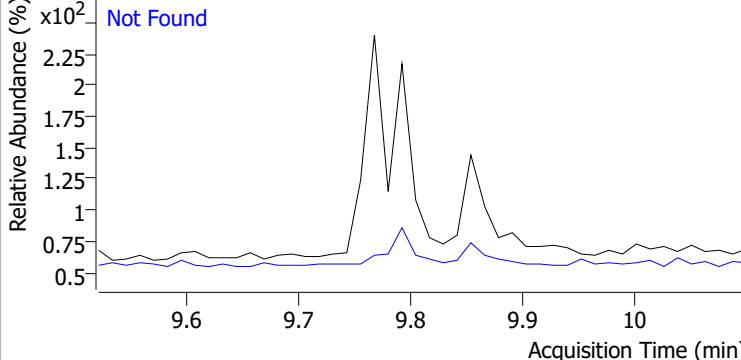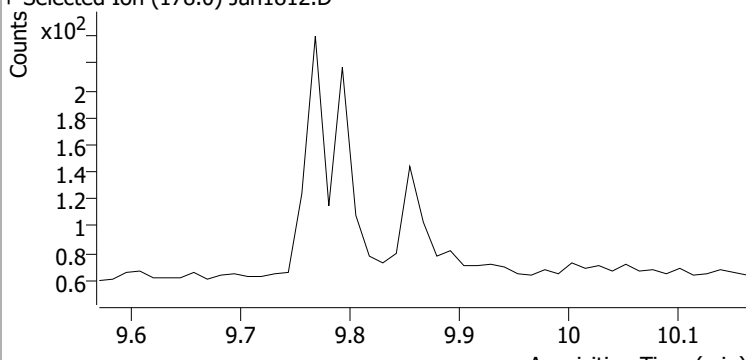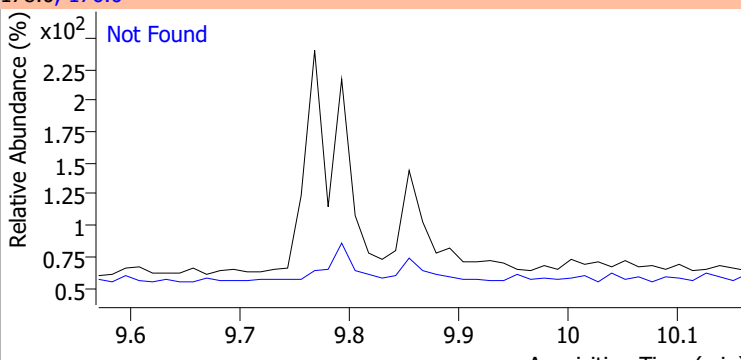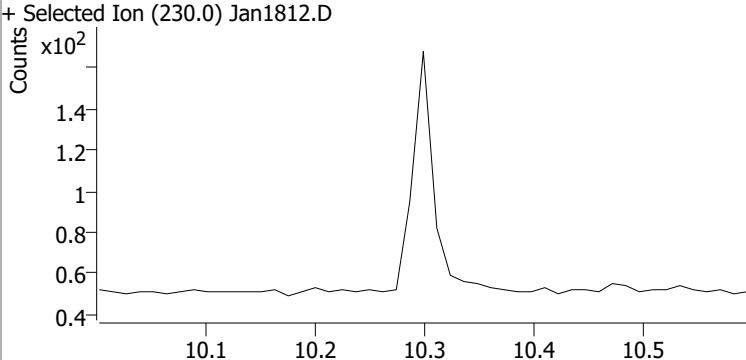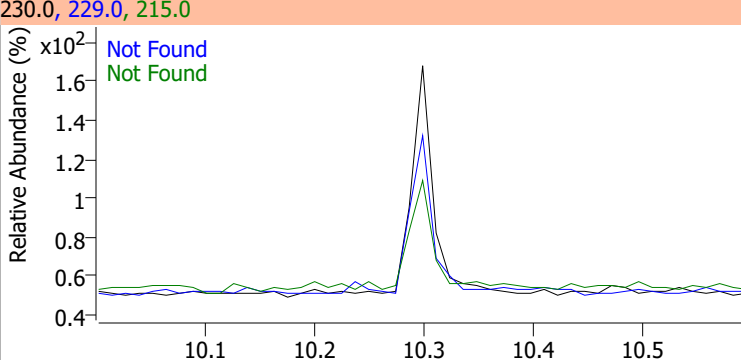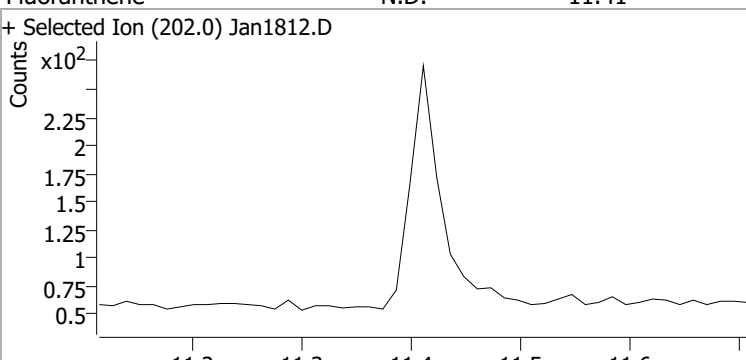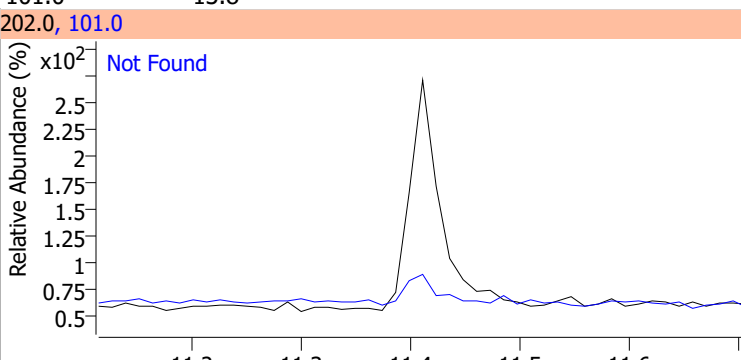
Compound	Conc.	Exp RT	QIon	Exp Ratio		
Phenanthrene	N.D.	9.80	176.0	15.5		
+ Selected Ion (178.0) Jan1812.D			178.0, 176.0			
						
Anthracene	N.D.	9.87	176.0	18.1		
+ Selected Ion (178.0) Jan1812.D			178.0, 176.0			
						
o-Terphenyl	N.D.	10.30	229.0	70.2	QIon	Exp Ratio
+ Selected Ion (230.0) Jan1812.D			230.0, 229.0, 215.0			
						
Fluoranthene	N.D.	11.41	101.0	13.8		
+ Selected Ion (202.0) Jan1812.D			202.0, 101.0			
						

Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.73	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.79	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.5	30.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.23	138.0	28.9




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.30	279.0	25.1	139.0	24.1




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.56	138.0	28.0	277.0	23.3



Quantitation Results Report (QT Reviewed)

Data File	Jan1813.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/18/2022 9:51:14 PM
Sample Name	B22010626-001C	Instrument	GCMS
Vial	13	Multiplier	1.00
DA Method File	011722 bna SIM 1.batch.bin	Comment	SVOC-8270C-SIM-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011822 bna SIM1.batch.bin	Last Calib Update	1/17/2022 8:49:06 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.484	152.0	180467	40.0000	ng/ml	-0.012
M Naphthalene-d8	5.928	136.0	328000	40.0000	ng/ml	-0.012
M Acenaphthene-d10	8.000	164.0	183102	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.768	188.0	364570	40.0000	ng/ml	-0.012
M Chrysene-d12	14.701	240.0	258742	40.0000	ng/ml	-0.025
M Perylene-d12	18.475	264.0	171930	40.0000	ng/ml	-0.025
System Monitoring Compounds						
S Nitrobenzene-d5	5.118	82.0	340454	35.7782	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 715.56%		*
S 2-Fluorobiphenyl	7.252	172.0	605736	68.8249	ng/ml	-0.012
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1376.50%		*
S o-Terphenyl	10.299	230.0	474	0.0798	ng/ml	0.000
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = 1.60%		*
S Terphenyl-d14	12.251	244.0	489096	71.3702	ng/ml	-0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 1427.40%		*
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.000	154.0	0		ng/ml	md 1
T Fluorene	8.960	166.0	0		ng/ml	md 1
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.701	228.0	0		ng/ml	md 1
T Chrysene	14.764	228.0	0		ng/ml	md 1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.475	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	35.7782	5.12	-0.02	340454	54.0	36.1	25.9	48.1
					128.0	33.7	25.6	47.6




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.95	102.0	19.9	129.0	11.0



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.79	142.0	140.8	115.0	59.7




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	113.1	115.0	67.8




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	68.8249	7.25	-0.01	605736	171.0	36.9	26.6	49.5




Compound	Conc.	Exp RT	QIon	Exp Ratio
Acenaphthylene	N.D.	7.83	153.0	12.8







Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	0	0	0	0	153.0 152.0	82.1 41.0	152.6 76.1	







Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene	0	0	0	0	165.0 167.0	69.1 9.7	128.3 18.0	



Quantitation Results Report (QT Reviewed)

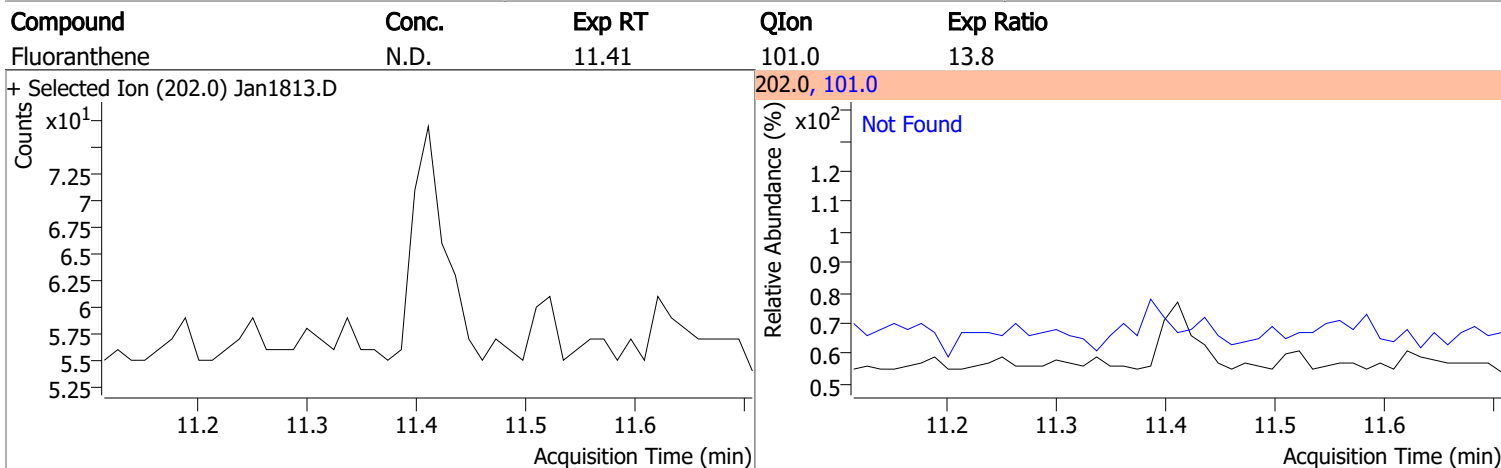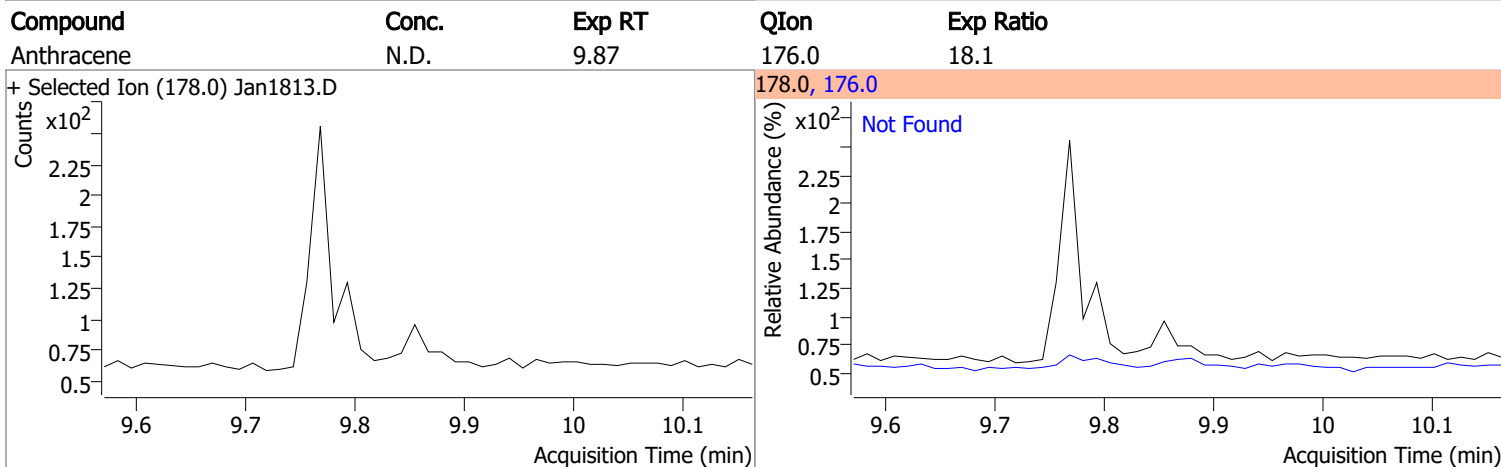


Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.73	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.79	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.5	30.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.23	138.0	28.9




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.30	279.0	25.1	139.0	24.1




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.56	138.0	28.0	277.0	23.3



Quantitation Results Report (QT Reviewed)

Data File	Jan1814.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/18/2022 10:23:36 PM
Sample Name	B22010628-001C	Instrument	GCMS
Vial	14	Multiplier	1.00
DA Method File	011722 bna SIM 1.batch.bin	Comment	SVOC-8270C-SIM-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011822 bna SIM1.batch.bin	Last Calib Update	1/17/2022 8:49:06 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.484	152.0	184199	40.0000	ng/ml	-0.012
M Naphthalene-d8	5.928	136.0	336442	40.0000	ng/ml	-0.012
M Acenaphthene-d10	8.000	164.0	188757	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.768	188.0	374008	40.0000	ng/ml	-0.012
M Chrysene-d12	14.714	240.0	254751	40.0000	ng/ml	-0.012
M Perylene-d12	18.475	264.0	170457	40.0000	ng/ml	-0.025
System Monitoring Compounds						
S Nitrobenzene-d5	5.118	82.0	359271	36.4967	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 729.93%		*
S 2-Fluorobiphenyl	7.252	172.0	518904	57.1923	ng/ml	-0.012
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1143.85%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.263	244.0	514783	75.0413	ng/ml	0.000
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 1500.83%		*
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.000	154.0	0		ng/ml	md
T Fluorene	8.973	166.0	0		ng/ml	md
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.701	228.0	0		ng/ml	md
T Chrysene	14.701	228.0	0		ng/ml	md
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.475	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	36.4967	5.12	-0.02	359271	54.0	36.1	25.9	48.1
					128.0	31.9	25.6	47.6




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.95	102.0	19.9	129.0	11.0







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.79	142.0	140.8	115.0	59.7







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	113.1	115.0	67.8







Quantitation Results Report (QT Reviewed)



Quantitation Results Report (QT Reviewed)

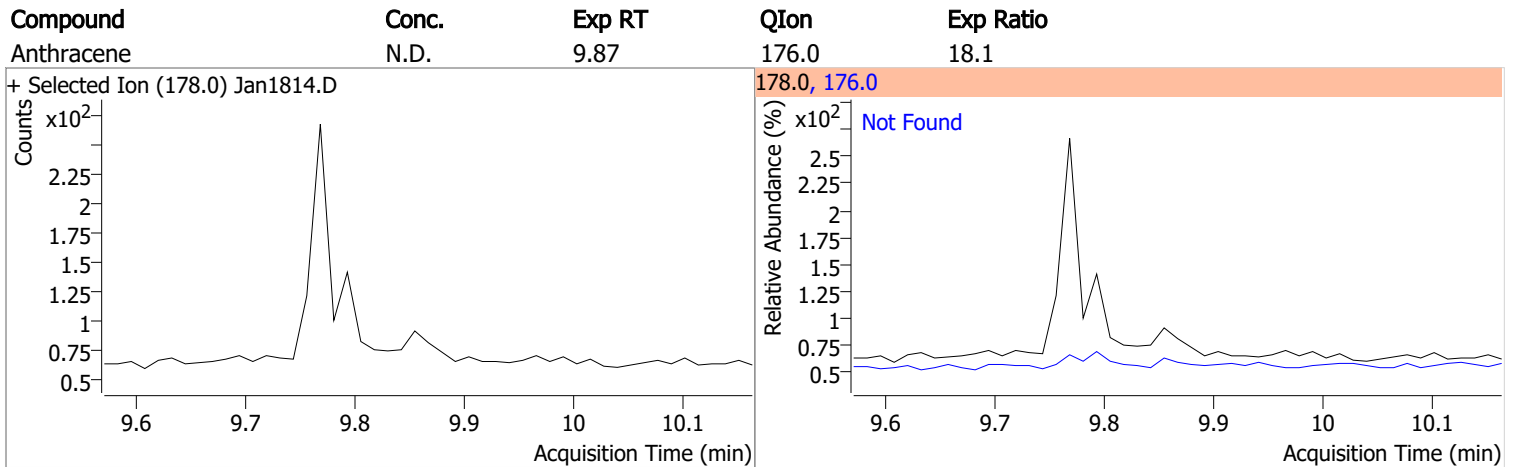


Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.73	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.79	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.5	30.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.23	138.0	28.9




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.30	279.0	25.1	139.0	24.1




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.56	138.0	28.0	277.0	23.3



Quantitation Results Report (QT Reviewed)

Data File	Jan1815.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/18/2022 10:55:51 PM
Sample Name	B22010628-001CLMS	Instrument	GCMS
Vial	15	Multiplier	1.00
DA Method File	011722 bna SIM 1.batch.bin	Comment	SVOC-8270C-SIM-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011822 bna SIM1.batch.bin	Last Calib Update	1/17/2022 8:49:06 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.484	152.0	179983	40.0000	ng/ml	-0.012
M Naphthalene-d8	5.928	136.0	340620	40.0000	ng/ml	-0.012
M Acenaphthene-d10	8.000	164.0	189254	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.768	188.0	374186	40.0000	ng/ml	-0.012
M Chrysene-d12	14.714	240.0	256534	40.0000	ng/ml	-0.012
M Perylene-d12	18.475	264.0	177004	40.0000	ng/ml	-0.025
System Monitoring Compounds						
S Nitrobenzene-d5	5.118	82.0	21726	5.3642	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 107.28%	*	
S 2-Fluorobiphenyl	7.252	172.0	40060	4.4037	ng/ml	-0.012
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 88.07%		
S o-Terphenyl	10.299	230.0	25020	4.1083	ng/ml	0.000
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = 82.17%		
S Terphenyl-d14	12.251	244.0	32588	6.7675	ng/ml	-0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 135.35%	*	
Target Compounds						
T Naphthalene	5.941	128.0	35850	3.0422	ng/ml	98
T 2-Methylnaphthalene	6.777	141.0	25530	3.8815	ng/ml	96
T 1-Methylnaphthalene	6.890	141.0	20289	2.9247	ng/ml	m 94
T Acenaphthylene	7.826	152.0	39931	3.4429	ng/ml	98
T Acenaphthene	8.038	154.0	26340	3.5503	ng/ml	96
T Fluorene	8.661	166.0	35740	4.0712	ng/ml	99
T Phenanthrene	9.793	178.0	54909	4.7335	ng/ml	92
T Anthracene	9.854	178.0	49701	4.7947	ng/ml	99
T Fluoranthene	11.398	202.0	57041	4.4947	ng/ml	99
T Pyrene	11.781	202.0	58999	4.5653	ng/ml	98
T Benzo(a)Anthracene	14.677	228.0	41902	5.0988	ng/ml	99
T Chrysene	14.776	228.0	56007	4.7701	ng/ml	98
T Benzo(b)fluoranthene	17.708	252.0	39526	4.9565	ng/ml	99


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	17.770	252.0	42330	4.5549	ng/ml	99
T Benzo(a)pyrene	18.351	252.0	31090	4.7991	ng/ml	99
T Indeno(1,2,3-cd)pyrene	20.204	276.0	28091	4.5442	ng/ml	100
T Dibenzo(a,h)anthracene	20.278	278.0	33509	4.7389	ng/ml	98
T Benzo(g,h,i)perylene	20.538	276.0	40760	4.6327	ng/ml	98


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	5.3642	5.12	-0.02	21726	54.0	34.9	25.9	48.1
					128.0	26.2	25.6	47.6



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	3.0422	5.94	-0.01	35850	102.0	18.5	0.0	59.6
					129.0	11.1	7.7	14.3




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	3.8815	6.78	-0.01	25530	142.0	144.6	98.5	183.0
					115.0	54.3	41.8	77.6




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	2.9247	6.89	-0.01	20289 (m)	142.0	121.4	79.2	147.1
					115.0	66.1	47.5	88.2




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	4.4037	7.25	-0.01	40060	171.0	35.8	26.6	49.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthylene	3.4429	7.83	0.00	39931	153.0	13.4	9.0	16.6






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	3.5503	8.04	0.00	26340	153.0	112.6	82.1	152.6
					152.0	56.9	41.0	76.1






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene	4.0712	8.66	-0.01	35740	165.0	97.5	69.1	128.3
					167.0	13.6	9.7	18.0






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Phenanthrene	4.7335	9.79	-0.01	54909	176.0	19.0	10.8	20.1



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Anthracene	4.7947	9.85	-0.01	49701	176.0	18.6	12.7	23.5




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
o-Terphenyl	4.1083	10.30	0.00	25020	229.0	69.0	49.2	91.3
					215.0	44.8	32.7	60.7




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluoranthene	4.4947	11.40	-0.01	57041	101.0	13.2	9.6	17.9




Pyrene	4.5653	11.78	-0.01	58999	101.0	16.0	10.7	20.0
--------	--------	-------	-------	-------	-------	------	------	------



Terphenyl-d14	6.7675	12.25	-0.01	32588	122.0	19.6	13.4	25.0
---------------	--------	-------	-------	-------	-------	------	------	------




Benzo(a)Anthracene	5.0988	14.68	-0.02	41902	226.0 229.0	27.5 22.3	18.9 16.1	35.1 29.9
--------------------	--------	-------	-------	-------	----------------	--------------	--------------	--------------




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	4.7701	14.78	-0.01	56007	226.0	30.3	21.2	39.4
					229.0	19.5	15.0	27.8




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(b)fluoranthene	4.9565	17.71	-0.02	39526	253.0	22.0	15.8	29.4



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(k)fluoranthene	4.5549	17.77	-0.02	42330	253.0	22.5	16.1	29.9



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene	4.7991	18.35	-0.02	31090	253.0	23.2	16.5	30.6




Quantitation Results Report (QT Reviewed)

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Indeno(1,2,3-cd)pyrene	4.5442	20.20	-0.02	28091	138.0	28.9	20.3	37.6
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1815.D</p> </div> <div style="width: 30%;"> <p>276.0, 138.0</p> <p>Ratio = 28.9 (99.8 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.204-20.204 min, 1 scans) (**) Jan1815.D</p> <p>Lib Match Score=78.5</p> </div> </div>								
Dibenzo(a,h)anthracene	4.7389	20.28	-0.02	33509	279.0	25.1	17.6	32.7
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (278.0) Jan1815.D</p> </div> <div style="width: 30%;"> <p>278.0, 279.0, 139.0</p> <p>Ratio = 25.1 (100.0 %)</p> <p>Ratio = 22.1 (91.7 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.278-20.278 min, 1 scans) (**) Jan1815.D</p> <p>Lib Match Score=77.8</p> </div> </div>								
Benzo(g,h,i)perylene	4.6327	20.54	-0.02	40760	138.0	27.2	19.6	36.5
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1815.D</p> </div> <div style="width: 30%;"> <p>276.0, 138.0, 277.0</p> <p>Ratio = 27.2 (97.1 %)</p> <p>Ratio = 24.5 (105.4 %)</p> </div> <div style="width: 30%;"> <p>+ SIM (20.538-20.538 min, 1 scans) (**) Jan1815.D</p> <p>Lib Match Score=78.6</p> </div> </div>								

Quantitation Results Report (QT Reviewed)

Data File	Jan1816.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/18/2022 11:28:13 PM
Sample Name	B22010629-001C	Instrument	GCMS
Vial	16	Multiplier	1.00
DA Method File	011722 bna SIM 1.batch.bin	Comment	SVOC-8270C-SIM-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011822 bna SIM1.batch.bin	Last Calib Update	1/17/2022 8:49:06 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.484	152.0	187207	40.0000	ng/ml	-0.012
M Naphthalene-d8	5.928	136.0	336020	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.000	164.0	187279	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.768	188.0	358196	40.0000	ng/ml	-0.012
M Chrysene-d12	14.714	240.0	256511	40.0000	ng/ml	-0.012
M Perylene-d12	18.474	264.0	172622	40.0000	ng/ml	-0.025
System Monitoring Compounds						
S Nitrobenzene-d5	5.118	82.0	272202	30.5734	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 611.47%		*
S 2-Fluorobiphenyl	7.252	172.0	471607	52.3896	ng/ml	-0.013
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1047.79%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.251	244.0	501315	73.1848	ng/ml	-0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 1463.70%		*
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.000	154.0	0		ng/ml	md
T Fluorene	8.960	166.0	0		ng/ml	md
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.701	228.0	0		ng/ml	md
T Chrysene	14.701	228.0	0		ng/ml	md
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.474	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	30.5734	5.12	-0.02	272202	54.0	35.7	25.9	48.1
					128.0	32.9	25.6	47.6




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.95	102.0	19.9	129.0	11.0







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.79	142.0	140.8	115.0	59.7







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	113.1	115.0	67.8







Quantitation Results Report (QT Reviewed)

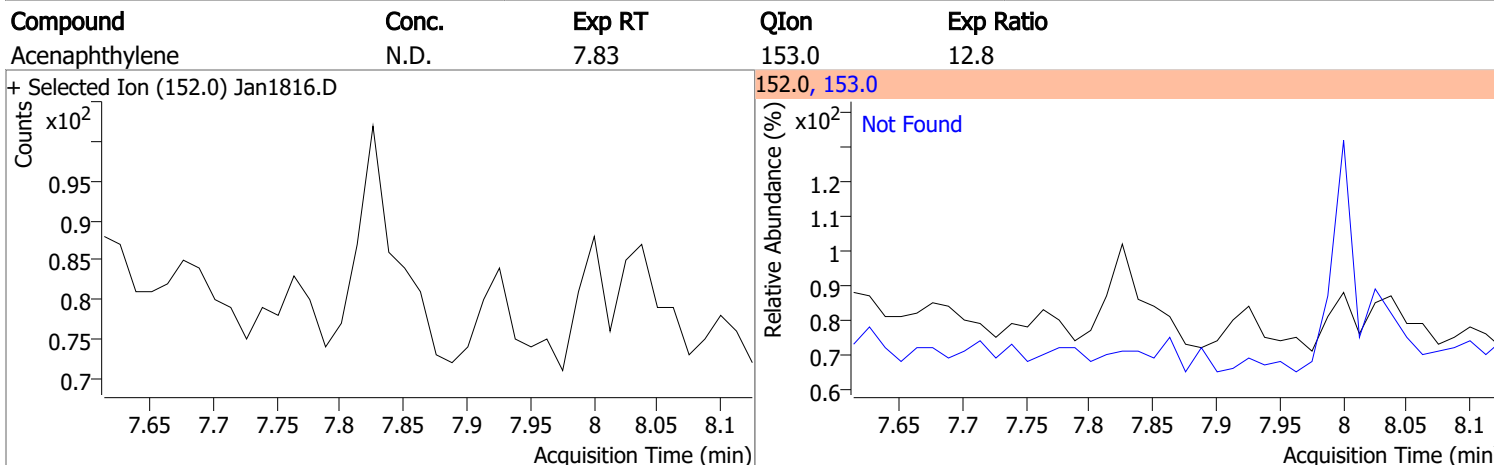





Quantitation Results Report (QT Reviewed)

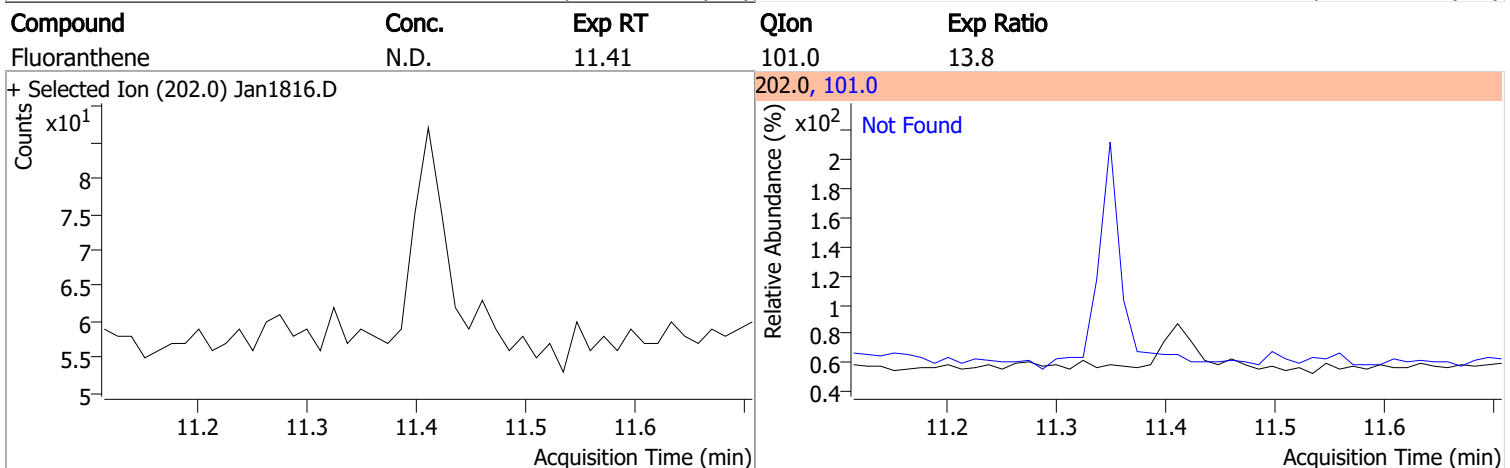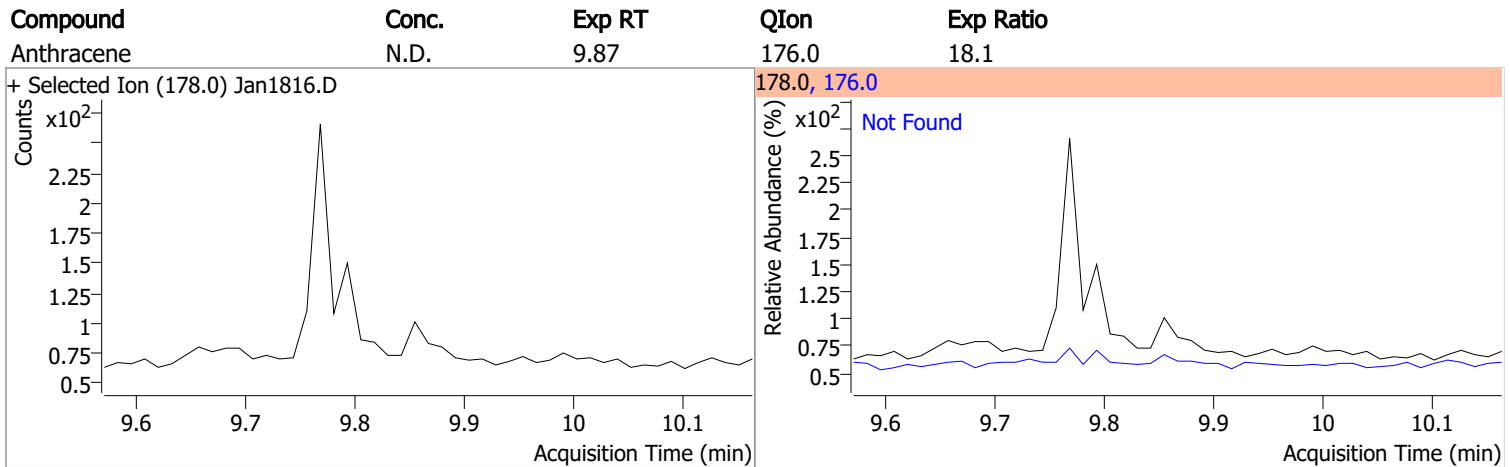

Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)

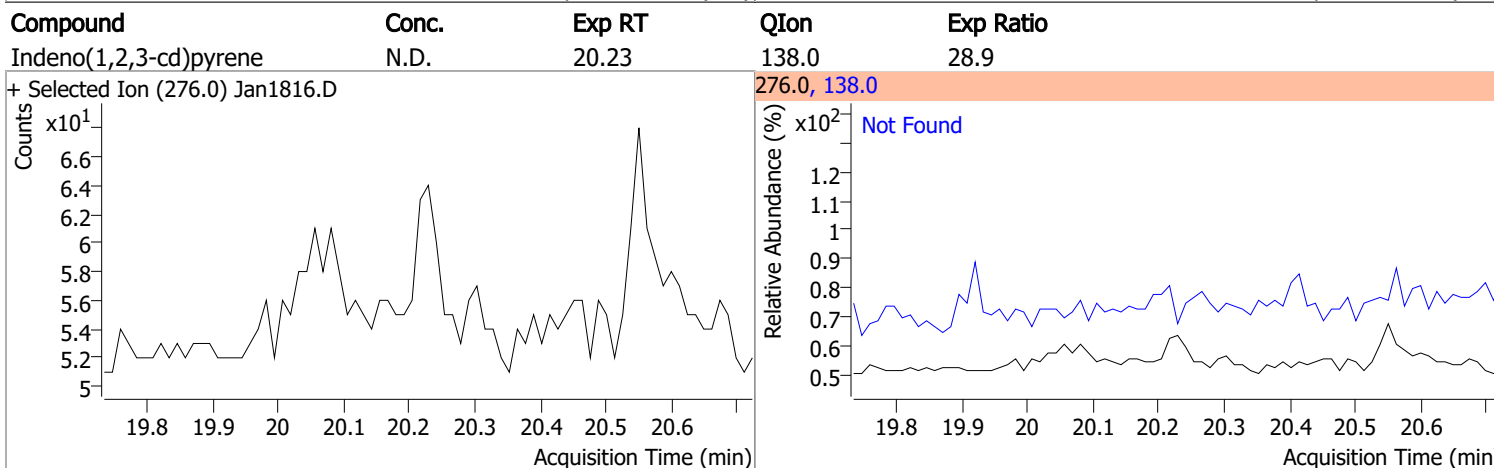


Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.30	279.0	25.1	139.0	24.1




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.56	138.0	28.0	277.0	23.3



Quantitation Results Report (QT Reviewed)

Data File	Jan1817.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/19/2022 12:00:24 AM
Sample Name	B22010633-001C	Instrument	GCMS
Vial	17	Multiplier	1.00
DA Method File	011722 bna SIM 1.batch.bin	Comment	SVOC-8270C-SIM-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011822 bna SIM1.batch.bin	Last Calib Update	1/17/2022 8:49:06 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.484	152.0	192081	40.0000	ng/ml	-0.012
M Naphthalene-d8	5.928	136.0	341792	40.0000	ng/ml	-0.012
M Acenaphthene-d10	8.001	164.0	195636	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.768	188.0	375780	40.0000	ng/ml	-0.012
M Chrysene-d12	14.714	240.0	260038	40.0000	ng/ml	-0.012
M Perylene-d12	18.475	264.0	175227	40.0000	ng/ml	-0.025
System Monitoring Compounds						
S Nitrobenzene-d5	5.118	82.0	325812	33.5672	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 671.34%		*
S 2-Fluorobiphenyl	7.252	172.0	554384	58.9546	ng/ml	-0.012
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1179.09%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.251	244.0	434947	65.0292	ng/ml	-0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 1300.58%		*
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.013	154.0	0		ng/ml	md 1
T Fluorene	8.960	166.0	0		ng/ml	md 1
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	11.411	202.0	659	0.0517	ng/ml	99
T Pyrene	11.781	202.0	811	0.0619	ng/ml	98
T Benzo(a)Anthracene	14.702	228.0	0		ng/ml	md 1
T Chrysene	14.776	228.0	402	0.0338	ng/ml	m 94
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.363	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	33.5672	5.12	-0.02	325812	54.0	35.2	25.9	48.1
					128.0	32.9	25.6	47.6




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.95	102.0	19.9	129.0	11.0







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.79	142.0	140.8	115.0	59.7







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	113.1	115.0	67.8







Quantitation Results Report (QT Reviewed)



Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.73	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.79	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.5	30.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.23	138.0	28.9




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.30	279.0	25.1	139.0	24.1



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.56	138.0	28.0	277.0	23.3




Quantitation Results Report (QT Reviewed)

Data File Jan1818.D
 Acq. Method 5975BNASIM
 Sample Name B22010633-001CLMS
 Vial 18
 DA Method File 011722 bna SIM 1.batch.bin
 Tune File dftppjph.u
 Batch Name 011822 bna SIM1.batch.bin

Operator LIMS import
 Acq. Date-Time 1/19/2022 12:32:39 AM
 Instrument GCMS
 Multiplier 1.00
 Comment SVOC-8270C-SIM-W-LLPAH
 Tune Date
 Last Calib Update 1/17/2022 8:49:06 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.484	152.0	182639	40.0000	ng/ml	-0.012
M Naphthalene-d8	5.928	136.0	330282	40.0000	ng/ml	-0.012
M Acenaphthene-d10	8.001	164.0	187686	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.768	188.0	370851	40.0000	ng/ml	-0.012
M Chrysene-d12	14.714	240.0	250431	40.0000	ng/ml	-0.012
M Perylene-d12	18.475	264.0	169126	40.0000	ng/ml	-0.025
System Monitoring Compounds						
S Nitrobenzene-d5	5.118	82.0	18854	4.7218	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%		Recovery = 94.44%			
S 2-Fluorobiphenyl	7.252	172.0	35960	3.9860	ng/ml	-0.012
Spiked Amount: 5.000	Range: 25.0 - 94.0%		Recovery = 79.72%			
S o-Terphenyl	10.299	230.0	24669	4.0872	ng/ml	0.000
Spiked Amount: 5.000	Range: 40.0 - 140.0%		Recovery = 81.74%			
S Terphenyl-d14	12.251	244.0	29248	6.2405	ng/ml	-0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%		Recovery = 124.81%		*	
Target Compounds						
T Naphthalene	5.941	128.0	30593	2.6774	ng/ml	99
T 2-Methylnaphthalene	6.777	141.0	21803	3.4187	ng/ml	91
T 1-Methylnaphthalene	6.890	141.0	18107	2.6920	ng/ml	96
T Acenaphthylene	7.826	152.0	35881	3.1195	ng/ml	97
T Acenaphthene	8.038	154.0	23740	3.2265	ng/ml	98
T Fluorene	8.661	166.0	33231	3.8171	ng/ml	99
T Phenanthrene	9.793	178.0	52412	4.5620	ng/ml	91
T Anthracene	9.854	178.0	48123	4.6899	ng/ml	97
T Fluoranthene	11.398	202.0	56202	4.4684	ng/ml	98
T Pyrene	11.781	202.0	59114	4.6857	ng/ml	98
T Benzo(a)Anthracene	14.677	228.0	41515	5.1707	ng/ml	99
T Chrysene	14.776	228.0	54631	4.7663	ng/ml	99
T Benzo(b)fluoranthene	17.709	252.0	40304	5.2895	ng/ml	99


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	17.770	252.0	41718	4.6925	ng/ml	99
T Benzo(a)pyrene	18.351	252.0	30819	4.9599	ng/ml	100
T Indeno(1,2,3-cd)pyrene	20.204	276.0	29502	4.9445	ng/ml	97
T Dibenzo(a,h)anthracene	20.266	278.0	34997	5.1798	ng/ml	97
T Benzo(g,h,i)perylene	20.538	276.0	40912	4.8483	ng/ml	98


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	4.7218	5.12	-0.02	18854	54.0	35.3	25.9	48.1
					128.0	26.7	25.6	47.6



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	2.6774	5.94	-0.01	30593	102.0	19.0	0.0	59.6
					129.0	11.1	7.7	14.3






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	3.4187	6.78	-0.01	21803	142.0	150.2	98.5	183.0
					115.0	50.7	41.8	77.6






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	2.6920	6.89	-0.01	18107	142.0	116.3	79.2	147.1
					115.0	63.1	47.5	88.2






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	3.9860	7.25	-0.01	35960	171.0	36.2	26.6	49.5
					172.0	36.2	26.6	49.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthylene	3.1195	7.83	0.00	35881	153.0	14.0	9.0	16.6
					152.0	14.0	9.0	16.6






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	3.2265	8.04	0.00	23740	153.0	115.3	82.1	152.6
					152.0	59.6	41.0	76.1
					154.0	59.6	41.0	76.1






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene	3.8171	8.66	-0.01	33231	165.0	99.2	69.1	128.3
					167.0	13.4	9.7	18.0






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Phenanthrene	4.5620	9.79	-0.01	52412	176.0	19.1	10.8	20.1



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Anthracene	4.6899	9.85	-0.01	48123	176.0	16.7	12.7	23.5




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
o-Terphenyl	4.0872	10.30	0.00	24669	229.0	68.3	49.2	91.3
					215.0	45.4	32.7	60.7




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluoranthene	4.4684	11.40	-0.01	56202	101.0	13.1	9.6	17.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Pyrene	4.6857	11.78	-0.01	59114	101.0	16.2	10.7	20.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Terphenyl-d14	6.2405	12.25	-0.01	29248	122.0	19.9	13.4	25.0




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)Anthracene	5.1707	14.68	-0.02	41515	226.0	27.5	18.9	35.1
					229.0	22.2	16.1	29.9




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	4.7663	14.78	-0.01	54631	226.0	30.2	21.2	39.4
					229.0	20.6	15.0	27.8




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(b)fluoranthene	5.2895	17.71	-0.02	40304	253.0	21.9	15.8	29.4












Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(k)fluoranthene	4.6925	17.77	-0.02	41718	253.0	22.7	16.1	29.9



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene	4.9599	18.35	-0.02	30819	253.0	23.4	16.5	30.6




Quantitation Results Report (QT Reviewed)

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Indeno(1,2,3-cd)pyrene	4.9445	20.20	-0.02	29502	138.0	27.1	20.3	37.6
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1818.D</p>  </div> <div style="width: 30%;"> <p>276.0, 138.0</p> <p>Ratio = 27.1 (93.6 %)</p>  </div> <div style="width: 30%;"> <p>+ SIM (20.204-20.204 min, 1 scans) (**) Jan1818.D</p> <p>Lib Match Score=78.5</p>  </div> </div>								
Dibenzo(a,h)anthracene	5.1798	20.27	-0.04	34997	279.0	24.6	17.6	32.7
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (278.0) Jan1818.D</p>  </div> <div style="width: 30%;"> <p>278.0, 279.0, 139.0</p> <p>Ratio = 24.6 (97.8 %)</p> <p>Ratio = 21.7 (90.1 %)</p>  </div> <div style="width: 30%;"> <p>+ SIM (20.266-20.266 min, 1 scans) (**) Jan1818.D</p> <p>Lib Match Score=76.2</p>  </div> </div>								
Benzo(g,h,i)perylene	4.8483	20.54	-0.02	40912	138.0	27.1	19.6	36.5
<div style="display: flex; justify-content: space-between;"> <div style="width: 30%;"> <p>+ Selected Ion (276.0) Jan1818.D</p>  </div> <div style="width: 30%;"> <p>276.0, 138.0, 277.0</p> <p>Ratio = 27.1 (96.7 %)</p> <p>Ratio = 24.2 (103.9 %)</p>  </div> <div style="width: 30%;"> <p>+ SIM (20.538-20.538 min, 1 scans) (**) Jan1818.D</p> <p>Lib Match Score=78.5</p>  </div> </div>								

Quantitation Results Report (QT Reviewed)

Data File	Jan1819.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/19/2022 1:04:50 AM
Sample Name	B22010637-001C	Instrument	GCMS
Vial	19	Multiplier	1.00
DA Method File	011722 bna SIM 1.batch.bin	Comment	SVOC-8270C-SIM-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011822 bna SIM1.batch.bin	Last Calib Update	1/17/2022 8:49:06 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.484	152.0	199802	40.0000	ng/ml	-0.012
M Naphthalene-d8	5.928	136.0	331750	40.0000	ng/ml	-0.012
M Acenaphthene-d10	8.000	164.0	188715	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.768	188.0	371032	40.0000	ng/ml	-0.012
M Chrysene-d12	14.714	240.0	254490	40.0000	ng/ml	-0.012
M Perylene-d12	18.475	264.0	175850	40.0000	ng/ml	-0.025
System Monitoring Compounds						
S Nitrobenzene-d5	5.118	82.0	372701	35.5378	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 710.76%	*	
S 2-Fluorobiphenyl	7.252	172.0	595398	65.6382	ng/ml	-0.012
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1312.76%	*	
S o-Terphenyl	10.299	230.0	317	0.0526	ng/ml	0.000
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = 1.05%	*	
S Terphenyl-d14	12.251	244.0	510554	74.6364	ng/ml	-0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 1492.73%	*	
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.000	154.0	0		ng/ml	md 1
T Fluorene	8.960	166.0	0		ng/ml	md 1
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.701	228.0	0		ng/ml	md 1
T Chrysene	14.701	228.0	0		ng/ml	md 1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.475	252.0	0		ng/ml md	1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	35.5378	5.12	-0.02	372701	54.0	35.7	25.9	48.1
					128.0	31.3	25.6	47.6




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.95	102.0	19.9	129.0	11.0



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.79	142.0	140.8	115.0	59.7






Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	113.1	115.0	67.8





Quantitation Results Report (QT Reviewed)



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	65.6382	7.25	-0.01	595398	171.0	36.9	26.6	49.5





Compound	Conc.	Exp RT	QIon	Exp Ratio
Acenaphthylene	N.D.	7.83	153.0	12.8







Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	0	0	0	0	153.0 152.0	82.1 41.0	152.6 76.1	







Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene	0	0	0	0	165.0 167.0	69.1 9.7	128.3 18.0	







Quantitation Results Report (QT Reviewed)



Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)

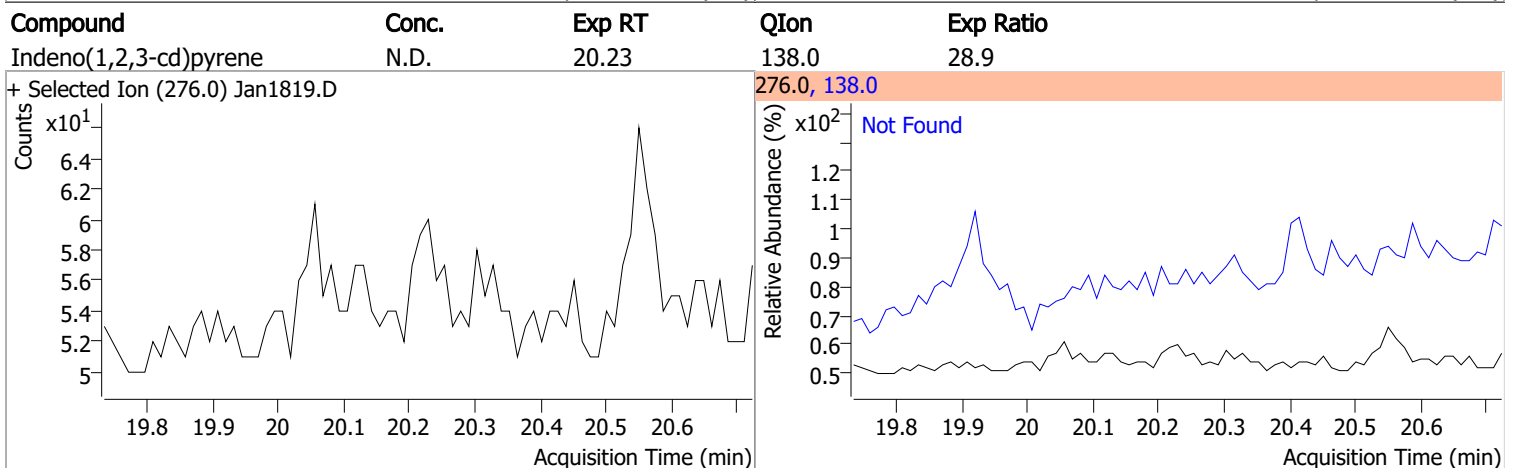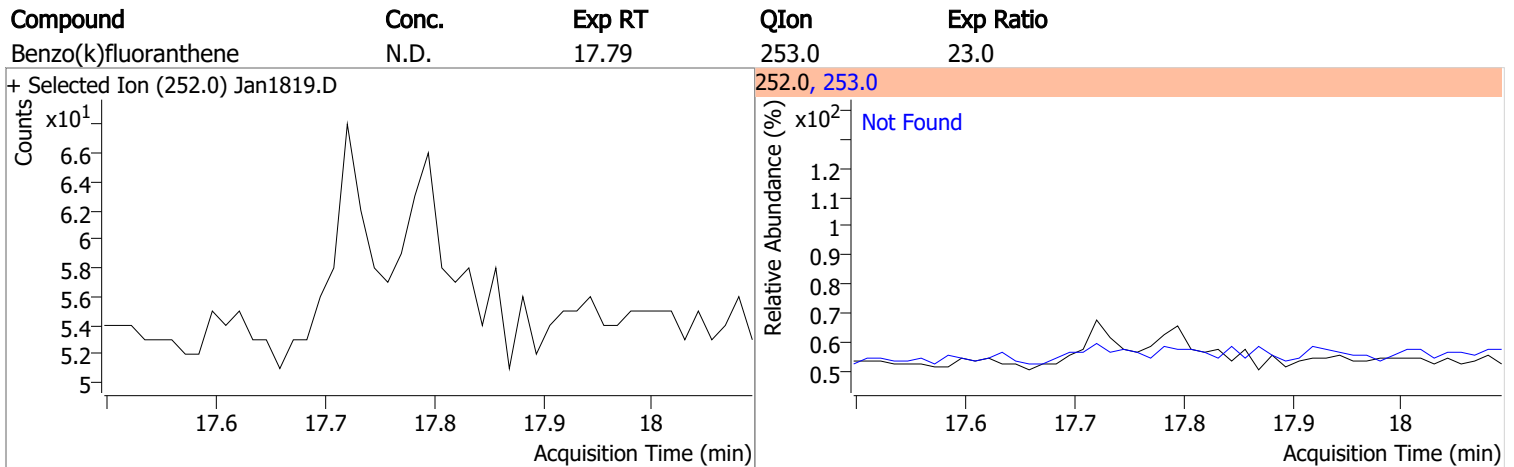


Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.30	279.0	25.1	139.0	24.1




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.56	138.0	28.0	277.0	23.3



Quantitation Results Report (QT Reviewed)

Data File	Jan1820.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/19/2022 1:37:05 AM
Sample Name	B22010641-001C	Instrument	GCMS
Vial	20	Multiplier	1.00
DA Method File	011722 bna SIM 1.batch.bin	Comment	SVOC-8270C-SIM-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011822 bna SIM1.batch.bin	Last Calib Update	1/17/2022 8:49:06 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.484	152.0	186457	40.0000	ng/ml	-0.012
M Naphthalene-d8	5.928	136.0	328639	40.0000	ng/ml	-0.012
M Acenaphthene-d10	8.001	164.0	187254	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.768	188.0	375309	40.0000	ng/ml	-0.012
M Chrysene-d12	14.702	240.0	257032	40.0000	ng/ml	-0.025
M Perylene-d12	18.475	264.0	172482	40.0000	ng/ml	-0.025
System Monitoring Compounds						
S Nitrobenzene-d5	5.118	82.0	374720	37.1523	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 743.05%	*	
S 2-Fluorobiphenyl	7.252	172.0	664650	73.8444	ng/ml	-0.012
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1476.89%	*	
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.251	244.0	530104	76.1952	ng/ml	-0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 1523.90%	*	
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.001	154.0	0		ng/ml	md 1
T Fluorene	8.973	166.0	0		ng/ml	md 1
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.702	228.0	0		ng/ml	md 1
T Chrysene	14.702	228.0	0		ng/ml	md 1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.475	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	37.1523	5.12	-0.02	374720	54.0	36.5	25.9	48.1
					128.0	33.3	25.6	47.6




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.95	102.0	19.9	129.0	11.0







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.79	142.0	140.8	115.0	59.7



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	113.1	115.0	67.8




Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Phenanthrene	N.D.	9.80	176.0	15.5




Compound	Conc.	Exp RT	QIon	Exp Ratio
Anthracene	N.D.	9.87	176.0	18.1







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
o-Terphenyl	N.D.	10.30	229.0	70.2	215.0	46.7







Compound	Conc.	Exp RT	QIon	Exp Ratio
Fluoranthene	N.D.	11.41	101.0	13.8



Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)

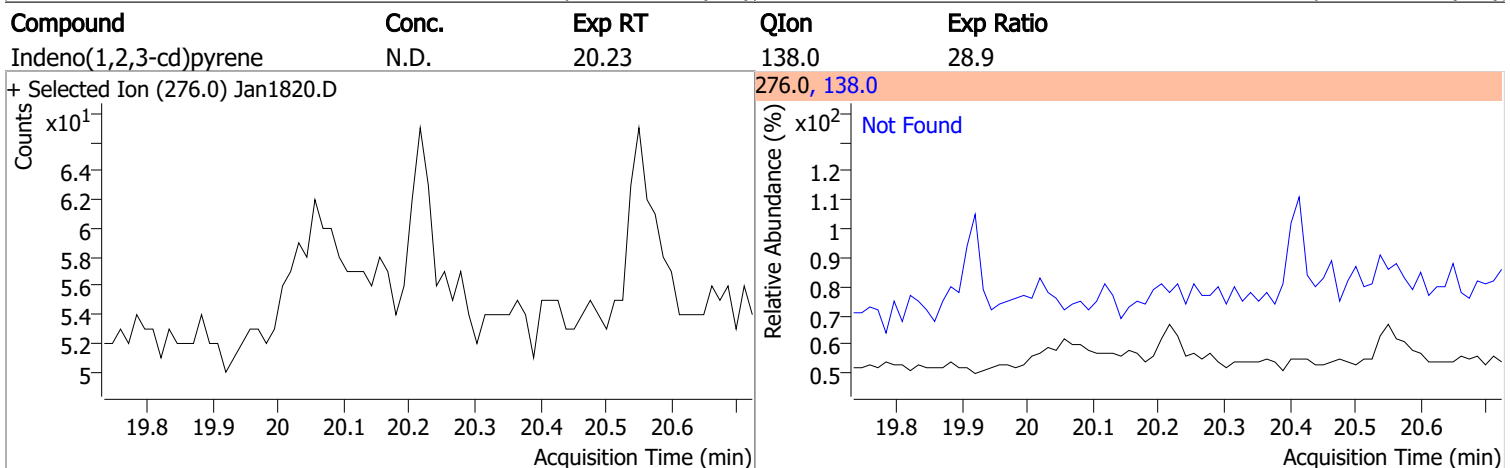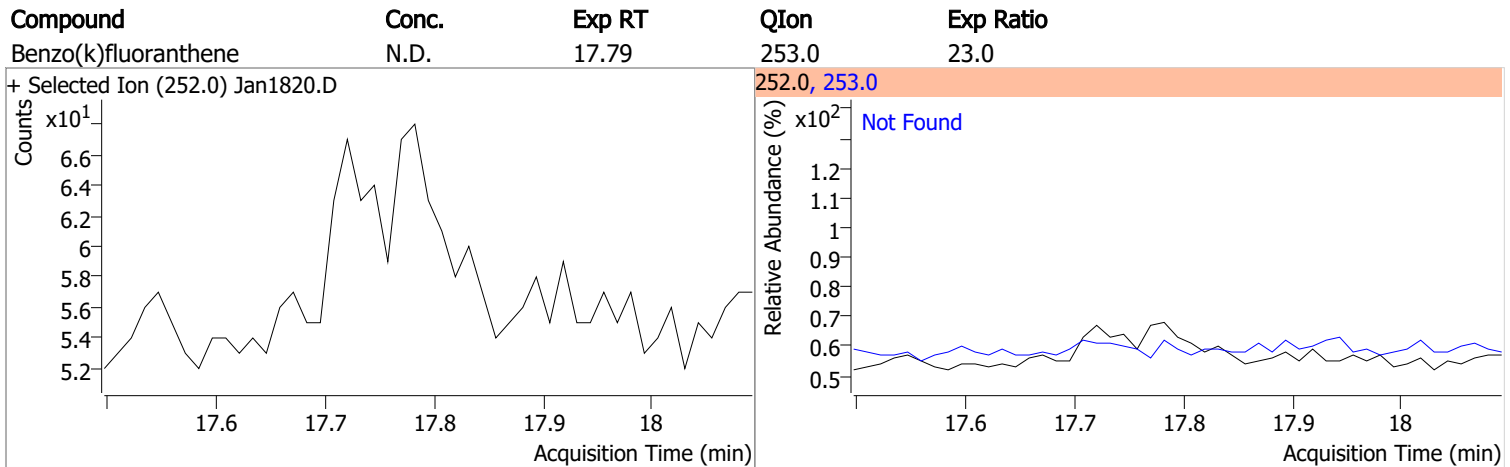


Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.30	279.0	25.1	139.0	24.1




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.56	138.0	28.0	277.0	23.3



Quantitation Results Report (QT Reviewed)

Data File	Jan1821.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/19/2022 2:09:15 AM
Sample Name	B22010643-001C	Instrument	GCMS
Vial	21	Multiplier	1.00
DA Method File	011722 bna SIM 1.batch.bin	Comment	SVOC-8270C-SIM-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011822 bna SIM1.batch.bin	Last Calib Update	1/17/2022 8:49:06 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.484	152.0	203390	40.0000	ng/ml	-0.012
M Naphthalene-d8	5.928	136.0	321307	40.0000	ng/ml	-0.012
M Acenaphthene-d10	8.001	164.0	211595	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.768	188.0	424186	40.0000	ng/ml	-0.012
M Chrysene-d12	14.714	240.0	284522	40.0000	ng/ml	-0.012
M Perylene-d12	18.475	264.0	191635	40.0000	ng/ml	-0.025
System Monitoring Compounds						
S Nitrobenzene-d5	5.118	82.0	394770	36.3907	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 727.81%		*
S 2-Fluorobiphenyl	7.252	172.0	611505	60.1241	ng/ml	-0.012
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1202.48%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.251	244.0	556717	73.2500	ng/ml	-0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 1465.00%		*
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.001	154.0	0		ng/ml	md 1
T Fluorene	8.973	166.0	0		ng/ml	md 1
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.702	228.0	0		ng/ml	md 1
T Chrysene	14.702	228.0	0		ng/ml	md 1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.475	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	36.3907	5.12	-0.02	394770	54.0	36.0	25.9	48.1
					128.0	30.1	25.6	47.6




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.95	102.0	19.9	129.0	11.0







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.79	142.0	140.8	115.0	59.7











Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	113.1	115.0	67.8







Quantitation Results Report (QT Reviewed)

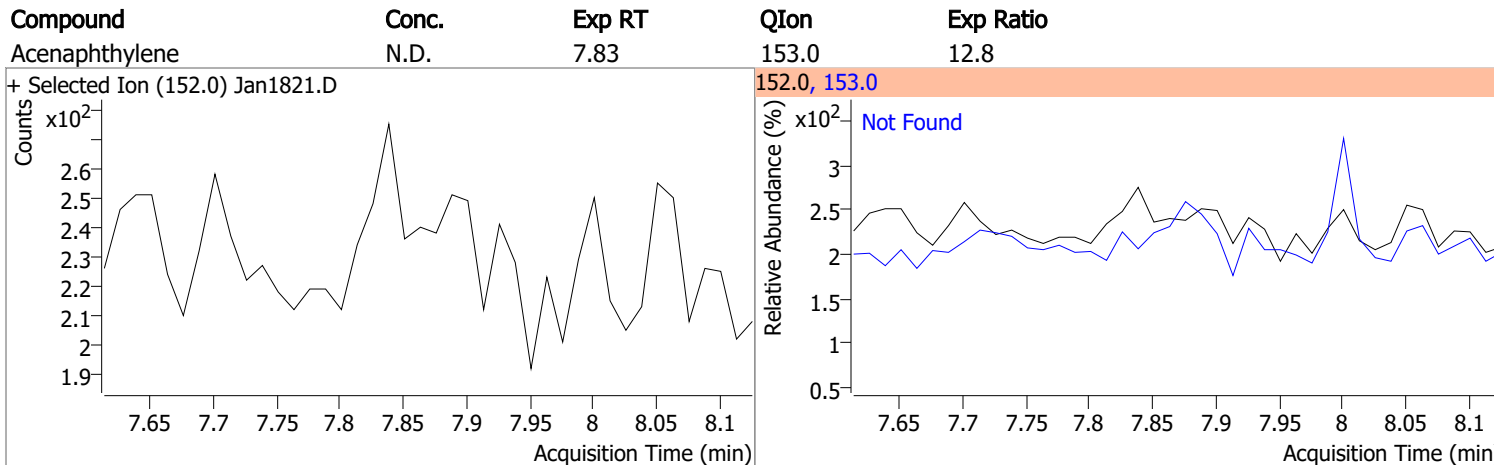

Quantitation Results Report (QT Reviewed)

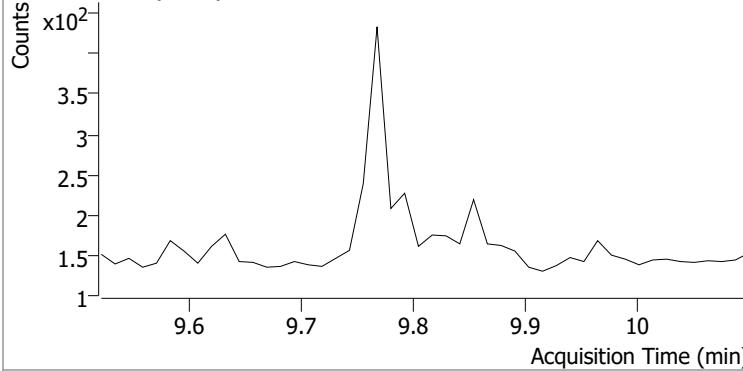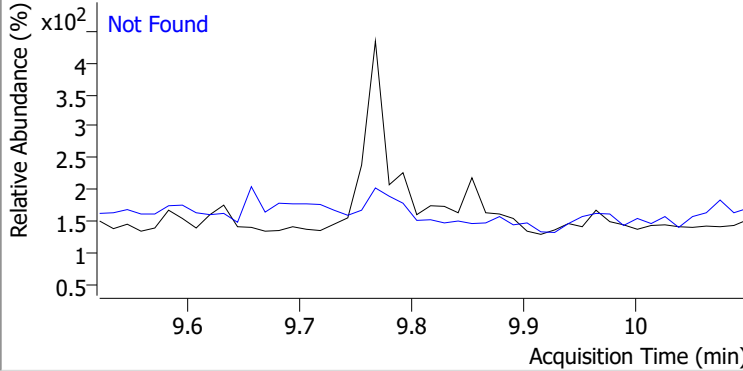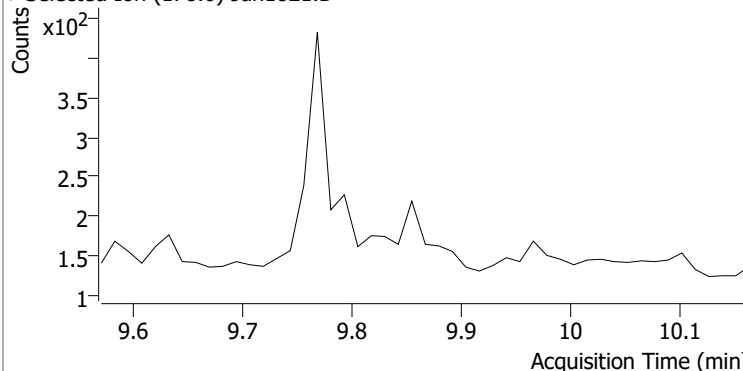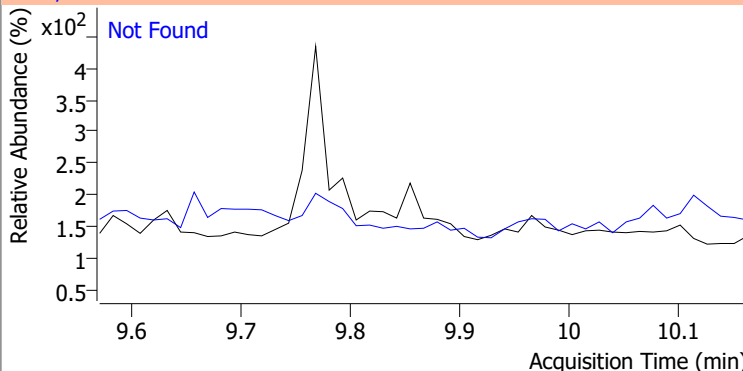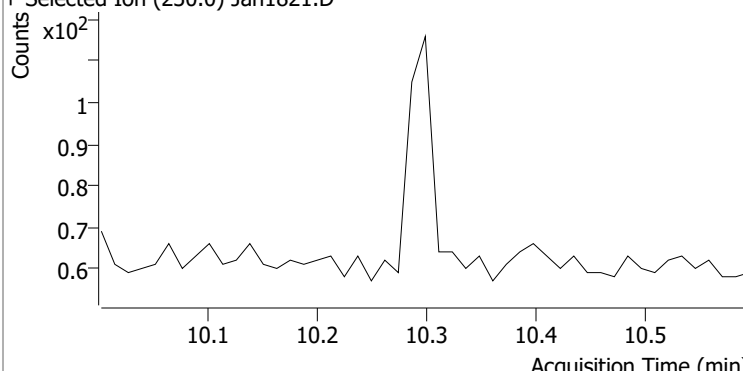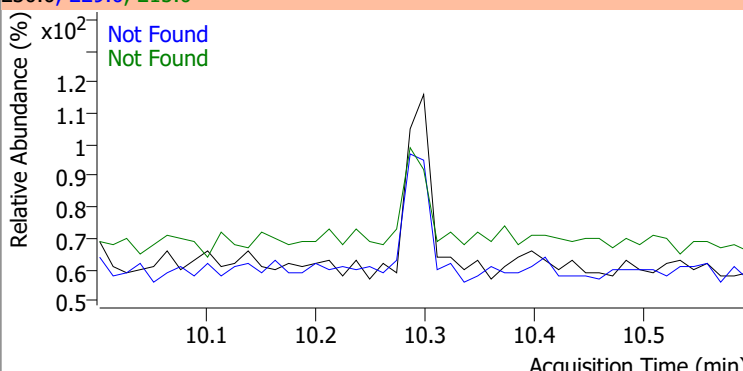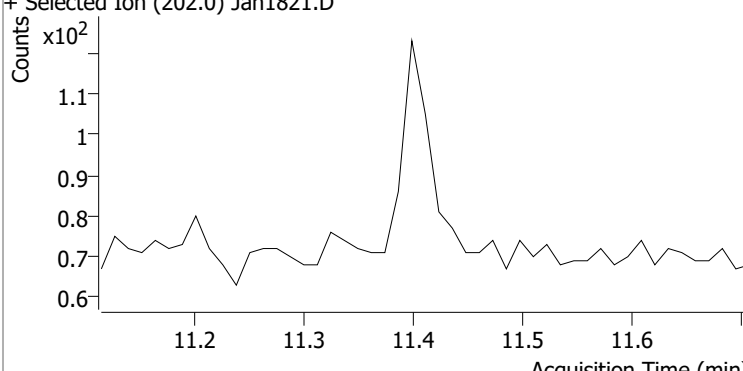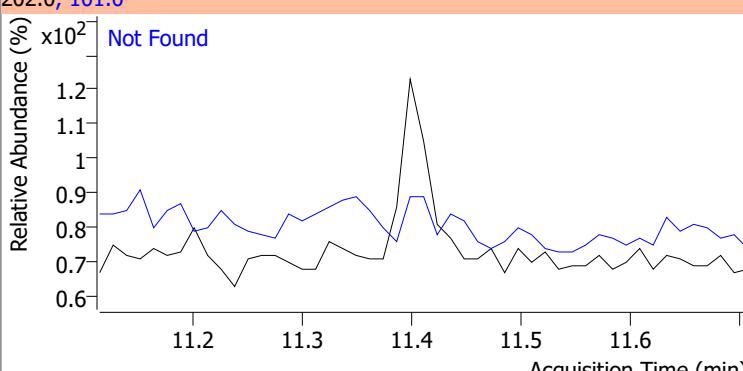
Compound	Conc.	Exp RT	QIon	Exp Ratio		
Phenanthrene	N.D.	9.80	176.0	15.5		
+ Selected Ion (178.0) Jan1821.D			178.0, 176.0			
						
Anthracene	N.D.	9.87	176.0	18.1		
+ Selected Ion (178.0) Jan1821.D			178.0, 176.0			
						
o-Terphenyl	N.D.	10.30	229.0	70.2	QIon	Exp Ratio
+ Selected Ion (230.0) Jan1821.D			230.0, 229.0, 215.0			
						
Fluoranthene	N.D.	11.41	101.0	13.8		
+ Selected Ion (202.0) Jan1821.D			202.0, 101.0			
						

Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.73	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.79	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.5	30.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.23	138.0	28.9




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.30	279.0	25.1	139.0	24.1




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.56	138.0	28.0	277.0	23.3



Quantitation Results Report (QT Reviewed)

Data File	Jan1822.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/19/2022 2:41:31 AM
Sample Name	B22010643-002A	Instrument	GCMS
Vial	22	Multiplier	1.00
DA Method File	011722 bna SIM 1.batch.bin	Comment	SVOC-8270C-SIM-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011822 bna SIM1.batch.bin	Last Calib Update	1/17/2022 8:49:06 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.484	152.0	198784	40.0000	ng/ml	-0.012
M Naphthalene-d8	5.928	136.0	346255	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.000	164.0	203071	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.768	188.0	414413	40.0000	ng/ml	-0.012
M Chrysene-d12	14.714	240.0	276063	40.0000	ng/ml	-0.012
M Perylene-d12	18.474	264.0	189978	40.0000	ng/ml	-0.025
System Monitoring Compounds						
S Nitrobenzene-d5	5.118	82.0	393503	36.8200	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 736.40%	*	
S 2-Fluorobiphenyl	7.252	172.0	550430	56.3909	ng/ml	-0.013
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1127.82%	*	
S o-Terphenyl	10.299	230.0	890	0.1320	ng/ml	0.000
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = 2.64%	*	
S Terphenyl-d14	12.250	244.0	524433	71.6380	ng/ml	-0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 1432.76%	*	
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	0.000		0	N.D.		
T Acenaphthene	8.000	154.0	0		ng/ml	md 1
T Fluorene	8.972	166.0	0		ng/ml	md 1
T Phenanthrene	0.000		0	N.D.		
T Anthracene	0.000		0	N.D.		
T Fluoranthene	0.000		0	N.D.		
T Pyrene	0.000		0	N.D.		
T Benzo(a)Anthracene	14.701	228.0	0		ng/ml	md 1
T Chrysene	14.701	228.0	0		ng/ml	md 1
T Benzo(b)fluoranthene	0.000		0	N.D.		


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	0.000		0	N.D.		
T Benzo(a)pyrene	18.474	252.0	0		ng/ml	md 1
T Indeno(1,2,3-cd)pyrene	0.000		0	N.D.		
T Dibenzo(a,h)anthracene	0.000		0	N.D.		
T Benzo(g,h,i)perylene	0.000		0	N.D.		


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	36.8200	5.12	-0.02	393503	54.0	36.5	25.9	48.1
					128.0	30.1	25.6	47.6




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.95	102.0	19.9	129.0	11.0







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.79	142.0	140.8	115.0	59.7







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	113.1	115.0	67.8







Quantitation Results Report (QT Reviewed)

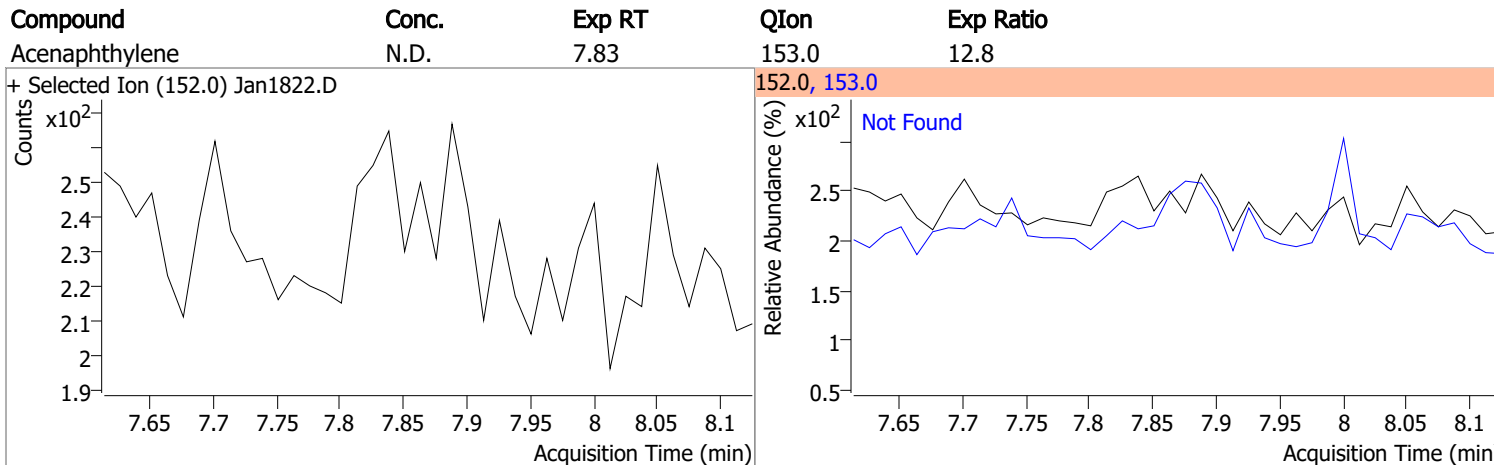

Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(b)fluoranthene	N.D.	17.73	253.0	22.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Benzo(k)fluoranthene	N.D.	17.79	253.0	23.0



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene		0		0	253.0		16.5	30.6




Compound	Conc.	Exp RT	QIon	Exp Ratio
Indeno(1,2,3-cd)pyrene	N.D.	20.23	138.0	28.9




Quantitation Results Report (QT Reviewed)

Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Dibenzo(a,h)anthracene	N.D.	20.30	279.0	25.1	139.0	24.1




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Benzo(g,h,i)perylene	N.D.	20.56	138.0	28.0	277.0	23.3



Quantitation Results Report (QT Reviewed)

Data File	Jan1823.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/19/2022 3:13:50 AM
Sample Name	B22010751-001C	Instrument	GCMS
Vial	23	Multiplier	1.00
DA Method File	011722 bna SIM 1.batch.bin	Comment	SVOC-8270C-SIM-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011822 bna SIM1.batch.bin	Last Calib Update	1/17/2022 8:49:06 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.484	152.0	205403	40.0000	ng/ml	-0.012
M Naphthalene-d8	5.928	136.0	360470	40.0000	ng/ml	-0.013
M Acenaphthene-d10	8.000	164.0	210031	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.768	188.0	413827	40.0000	ng/ml	-0.012
M Chrysene-d12	14.714	240.0	279463	40.0000	ng/ml	-0.012
M Perylene-d12	18.474	264.0	197998	40.0000	ng/ml	-0.025
System Monitoring Compounds						
S Nitrobenzene-d5	5.118	82.0	427590	37.9372	ng/ml	-0.025
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 758.74%		*
S 2-Fluorobiphenyl	7.252	172.0	635021	62.9014	ng/ml	-0.013
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 1258.03%		*
S o-Terphenyl	0.000		0	N.D.		
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = NA%		
S Terphenyl-d14	12.251	244.0	508345	69.3246	ng/ml	-0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 1386.49%		*
Target Compounds						
T Naphthalene	0.000		0	N.D.		
T 2-Methylnaphthalene	0.000		0	N.D.		
T 1-Methylnaphthalene	0.000		0	N.D.		
T Acenaphthylene	7.838	152.0	0		ng/ml	md 1
T Acenaphthene	8.075	154.0	0		ng/ml	md 1
T Fluorene	8.972	166.0	0		ng/ml	md 1
T Phenanthrene	9.793	178.0	0		ng/ml	md 1
T Anthracene	9.854	178.0	0		ng/ml	md 1
T Fluoranthene	11.398	202.0	1899	0.1353	ng/ml	94
T Pyrene	11.781	202.0	3780	0.2685	ng/ml	100
T Benzo(a)Anthracene	14.701	228.0	2622	0.1591	ng/ml	# 80
T Chrysene	14.776	228.0	1976	0.1545	ng/ml	94
T Benzo(b)fluoranthene	17.721	252.0	1726	0.1935	ng/ml	m 99


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	17.770	252.0	860	0.0747	ng/ml	92
T Benzo(a)pyrene	18.351	252.0	932	0.1254	ng/ml	90
T Indeno(1,2,3-cd)pyrene	20.204	276.0	697	0.1054	ng/ml m	98
T Dibenzo(a,h)anthracene	20.105	278.0	0		ng/ml md	1
T Benzo(g,h,i)perylene	20.538	276.0	1000	0.0859	ng/ml	95


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	37.9372	5.12	-0.02	427590	54.0	35.9	25.9	48.1
					128.0	30.4	25.6	47.6




Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
Naphthalene	N.D.	5.95	102.0	19.9	129.0	11.0







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
2-Methylnaphthalene	N.D.	6.79	142.0	140.8	115.0	59.7



Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
1-Methylnaphthalene	N.D.	6.90	142.0	113.1	115.0	67.8




Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Phenanthrene	0	0	0	0	176.0		10.8	20.1




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Anthracene	0	0	0	0	176.0		12.7	23.5







Compound	Conc.	Exp RT	QIon	Exp Ratio	QIon	Exp Ratio
o-Terphenyl	N.D.	10.30	229.0	70.2	215.0	46.7



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluoranthene	0.1353	11.40	-0.01	1899	101.0	11.4	9.6	17.9



Quantitation Results Report (QT Reviewed)




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(b)fluoranthene	0.1935	17.72	-0.01	1726 (m)	253.0	23.3	15.8	29.4
+ Selected Ion (252.0) Jan1823.D 			252.0, 253.0 			+ SIM (17.721-17.721 min, 1 scans) (**) Jan1823.D Lib Match Score=53.1 		
Benzo(k)fluoranthene	0.0747	17.77	-0.02	860	253.0	19.1	16.1	29.9
+ Selected Ion (252.0) Jan1823.D 			252.0, 253.0 			+ SIM (17.770-17.770 min, 1 scans) (**) Jan1823.D Lib Match Score=48.7 		
Benzo(a)pyrene	0.1254	18.35	-0.02	932	253.0	28.2	16.5	30.6
+ Selected Ion (252.0) Jan1823.D 			252.0, 253.0 			+ SIM (18.351-18.351 min, 1 scans) (**) Jan1823.D Lib Match Score=49.8 		
Indeno(1,2,3-cd)pyrene	0.1054	20.20	-0.02	697 (m)	138.0	30.0	20.3	37.6
+ Selected Ion (276.0) Jan1823.D 			276.0, 138.0 			+ SIM (20.204-20.204 min, 1 scans) (**) Jan1823.D Lib Match Score=54.9 		

Quantitation Results Report (QT Reviewed)

Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Dibenzo(a,h)anthracene		0		0	279.0		17.6	32.7
					139.0		16.9	31.3




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(g,h,i)perylene	0.0859	20.54	-0.02	1000	138.0	23.8	19.6	36.5
					277.0	24.5	16.3	30.2



Quantitation Results Report (QT Reviewed)

Data File	Jan1824.D	Operator	LIMS import
Acq. Method	5975BNASIM	Acq. Date-Time	1/19/2022 3:46:05 AM
Sample Name	18-Jan-22_CCV_24	Instrument	GCMS
Vial	24	Multiplier	1.00
DA Method File	011722 bna SIM 1.batch.bin	Comment	SVOC-8270C-SIM-W-LLPAH
Tune File	dftppjph.u	Tune Date	
Batch Name	011822 bna SIM1.batch.bin	Last Calib Update	1/17/2022 8:49:06 AM

Ref Library



Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
Internal Standards						
M 1,4-Dichlorobenzene-d4	4.484	152.0	169700	40.0000	ng/ml	-0.012
M Naphthalene-d8	5.928	136.0	306766	40.0000	ng/ml	-0.012
M Acenaphthene-d10	8.000	164.0	180613	40.0000	ng/ml	0.000
M Phenanthrene-d10	9.768	188.0	341465	40.0000	ng/ml	-0.012
M Chrysene-d12	14.701	240.0	244236	40.0000	ng/ml	-0.025
M Perylene-d12	18.475	264.0	166943	40.0000	ng/ml	-0.025
System Monitoring Compounds						
S Nitrobenzene-d5	5.131	82.0	6904	2.1144	ng/ml	-0.012
Spiked Amount: 5.000	Range: 19.0 - 102.0%			Recovery = 42.29%		
S 2-Fluorobiphenyl	7.252	172.0	14281	1.6450	ng/ml	-0.012
Spiked Amount: 5.000	Range: 25.0 - 94.0%			Recovery = 32.90%		
S o-Terphenyl	10.299	230.0	10023	1.8036	ng/ml	0.000
Spiked Amount: 5.000	Range: 40.0 - 140.0%			Recovery = 36.07%		*
S Terphenyl-d14	12.251	244.0	8940	1.9881	ng/ml	-0.012
Spiked Amount: 5.000	Range: 39.0 - 106.0%			Recovery = 39.76%		
Target Compounds						
T Naphthalene	5.941	128.0	18778	1.7693	ng/ml	99
T 2-Methylnaphthalene	6.777	141.0	11579	1.9547	ng/ml	99
T 1-Methylnaphthalene	6.890	141.0	11189	1.7910	ng/ml	96
T Acenaphthylene	7.826	152.0	17934	1.6203	ng/ml	98
T Acenaphthene	8.038	154.0	11801	1.6667	ng/ml	91
T Fluorene	8.661	166.0	14659	1.7497	ng/ml	100
T Phenanthrene	9.793	178.0	20961	1.9888	ng/ml	91
T Anthracene	9.854	178.0	18955	2.0590	ng/ml	99
T Fluoranthene	11.398	202.0	21638	1.8685	ng/ml	100
T Pyrene	11.781	202.0	22576	1.8349	ng/ml	96
T Benzo(a)Anthracene	14.677	228.0	15690	2.0183	ng/ml	99
T Chrysene	14.764	228.0	21260	1.9019	ng/ml	99
T Benzo(b)fluoranthene	17.709	252.0	14397	1.9141	ng/ml	99


Quantitation Results Report (QT Reviewed)

Compound	RT	QIon	Resp.	Conc.	Units	Dev(Min)
T Benzo(k)fluoranthene	17.770	252.0	15646	1.8241	ng/ml	98
T Benzo(a)pyrene	18.351	252.0	11515	2.0119	ng/ml	99
T Indeno(1,2,3-cd)pyrene	20.204	276.0	11185	2.0455	ng/ml	99
T Dibenzo(a,h)anthracene	20.279	278.0	11889	1.7827	ng/ml	99
T Benzo(g,h,i)perylene	20.538	276.0	14932	1.8816	ng/ml	97


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Nitrobenzene-d5	2.1144	5.13	-0.01	6904	54.0	38.3	25.9	48.1
					128.0	32.6	25.6	47.6



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Naphthalene	1.7693	5.94	-0.01	18778	102.0	20.4	0.0	59.6
					129.0	11.0	7.7	14.3




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Methylnaphthalene	1.9547	6.78	-0.01	11579	142.0	142.0	98.5	183.0
					115.0	61.3	41.8	77.6




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
1-Methylnaphthalene	1.7910	6.89	-0.01	11189	142.0 115.0	117.0 64.4	79.2 47.5	147.1 88.2




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
2-Fluorobiphenyl	1.6450	7.25	-0.01	14281	171.0	38.3	26.6	49.5



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthylene	1.6203	7.83	0.00	17934	153.0	13.5	9.0	16.6






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Acenaphthene	1.6667	8.04	0.00	11801	153.0 152.0	108.1 52.2	82.1 41.0	152.6 76.1






Quantitation Results Report (QT Reviewed)




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluorene	1.7497	8.66	-0.01	14659	165.0	99.1	69.1	128.3
					167.0	13.6	9.7	18.0






Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Phenanthrene	1.9888	9.79	-0.01	20961	176.0	19.3	10.8	20.1



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Anthracene	2.0590	9.85	-0.01	18955	176.0	18.5	12.7	23.5




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
o-Terphenyl	1.8036	10.30	0.00	10023	229.0	69.4	49.2	91.3
					215.0	45.1	32.7	60.7




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Fluoranthene	1.8685	11.40	-0.01	21638	101.0	13.7	9.6	17.9




Pyrene	1.8349	11.78	-0.01	22576	101.0	17.1	10.7	20.0
--------	--------	-------	-------	-------	-------	------	------	------



Terphenyl-d14	1.9881	12.25	-0.01	8940	122.0	20.2	13.4	25.0
---------------	--------	-------	-------	------	-------	------	------	------




Benzo(a)Anthracene	2.0183	14.68	-0.02	15690	226.0	27.1	18.9	35.1
					229.0	23.6	16.1	29.9




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Chrysene	1.9019	14.76	-0.02	21260	226.0 229.0	30.2 20.2	21.2 15.0	39.4 27.8




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(b)fluoranthene	1.9141	17.71	-0.02	14397	253.0	22.3	15.8	29.4



Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(k)fluoranthene	1.8241	17.77	-0.02	15646	253.0	23.9	16.1	29.9




Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Benzo(a)pyrene	2.0119	18.35	-0.02	11515	253.0	24.0	16.5	30.6




Quantitation Results Report (QT Reviewed)


Compound	Conc.	RT	Dev(Min)	Resp.	QIon	QRatio	Lower	Upper
Indeno(1,2,3-cd)pyrene	2.0455	20.20	-0.02	11185	138.0	28.2	20.3	37.6



Dibenzo(a,h)anthracene	1.7827	20.28	-0.02	11889	279.0	25.6	17.6	32.7
					139.0	24.0	16.9	31.3



Benzo(g,h,i)perylene	1.8816	20.54	-0.02	14932	138.0	29.3	19.6	36.5
					277.0	25.1	16.3	30.2



Continuing Calibration Report

Batch Name \\MASSHUNTER\Org\Data\SV5975.I\sh011822\1 e8270c bna SIM\QuantResults\011822 bna SIM1.batch.bin
Method File \\MASSHUNTER\Org\Data\SV5975.I\sh011722\1 e8270c bna SIM\011722 bna SIM 1.batch.bin
Daily CC \\MASSHUNTER\Org\Data\SV5975.I\sh011822\1 e8270c bna SIMJan1802.D

Level name	Injection Time	Calibration Files
7	1/14/2022 4:42:22 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1411.D
6	1/14/2022 5:14:49 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1412.D
5	1/14/2022 5:47:16 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1413.D
4	1/14/2022 6:19:44 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1414.D
3	1/14/2022 6:52:13 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1415.D
2	1/14/2022 7:24:38 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1416.D
1	1/14/2022 7:57:03 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1417.D
CCV	1/18/2022 3:55:24 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh011822\1 e8270c bna SIM\Jan1802.D <=====

ISTD Compound:	Avg Resp	Mid Resp	CC Resp	Area%	A/M
1,4-Dichlorobenzene-d4	173591	173466	185938	107.19	M
Naphthalene-d8	313667	320346	338631	105.71	M
Acenaphthene-d10	169911	171827	186457	108.51	M
Phenanthrene-d10	347083	351005	381095	108.57	M
Chrysene-d12	256387	261208	260043	99.55	M
Perylene-d12	167073	172756	176150	101.97	M

Target Compound	AvgRF/R2	CC RF	Exp. Conc	Calc. Conc	%Dev	Area%	Curve Fit
1,4-Dichlorobenzene-d4	-----ISTD-----						
Nitrobenzene-d5	0.9999	0.6953	2.00	1.83	8.30	96.49	Quadratic
Naphthalene-d8	-----ISTD-----						
Naphthalene	1.3839	1.1533	2.00	1.67	-16.66	92.74	Avg RF
2-Methylnaphthalene	0.7724	0.7357	2.00	1.90	-4.75	101.37	Avg RF
1-Methylnaphthalene	0.8146	0.7509	2.00	1.84	-7.83	105.25	Avg RF
Acenaphthene-d10	-----ISTD-----						
2-Fluorobiphenyl	1.9227	1.8701	2.00	1.95	-2.73	110.18	Avg RF
Acenaphthylene	2.4514	2.2005	2.00	1.80	-10.23	102.55	Avg RF
Acenaphthene	1.5681	1.3357	2.00	1.70	-14.82	96.51	Avg RF
Fluorene	1.8554	1.7133	2.00	1.85	-7.66	104.06	Avg RF
Phenanthrene-d10	-----ISTD-----						
Phenanthrene	0.9999	1.1922	2.00	1.93	3.46	102.26	Quadratic
Anthracene	0.9999	1.0851	2.00	2.01	-0.65	107.13	Quadratic
o-Terphenyl	0.6510	0.5949	2.00	1.83	-8.62	101.37	Avg RF
Fluoranthene	1.3566	1.2194	2.00	1.80	-10.12	102.00	Avg RF
Chrysene-d12	-----ISTD-----						
Pyrene	2.0151	2.0206	2.00	2.01	0.27	100.67	Avg RF
Terphenyl-d14	0.9999	0.7585	2.00	2.06	-3.00	100.00	Quadratic
Benzo(a)Anthracene	0.9998	1.3485	2.00	2.12	-6.12	103.09	Quadratic
Chrysene	1.8307	1.6812	2.00	1.84	-8.17	95.81	Avg RF
Perylene-d12	-----ISTD-----						
Benzo(b)fluoranthene	1.8021	1.6504	2.00	1.83	-8.42	92.37	Avg RF
Benzo(k)fluoranthene	0.9995	2.0384	2.00	1.98	0.92	100.79	Quadratic
Benzo(a)pyrene	0.9999	1.4507	2.00	2.11	-5.56	106.93	Quadratic
Indeno(1,2,3-cd)pyrene	0.9998	1.3129	2.00	2.01	-0.31	99.35	Quadratic
Dibenzo(a,h)anthracene	1.5980	1.4548	2.00	1.82	-8.96	101.94	Avg RF
Benzo(g,h,i)perylene	0.9998	1.8549	2.00	1.95	2.53	97.97	Quadratic

A -- against Average; M -- against Mid Point; P -- against Previous CC in the Method;

Continuing Calibration Report

Batch Name \\MASSHUNTER\Org\Data\SV5975.I\sh011822\1 e8270c bna SIM\QuantResults\011822 bna SIM1.batch.bin
Method File \\MASSHUNTER\Org\Data\SV5975.I\sh011722\1 e8270c bna SIM\011722 bna SIM 1.batch.bin
Daily CC \\MASSHUNTER\Org\Data\SV5975.I\sh011822\1 e8270c bna SIMJan1824.D

Level name	Injection Time	Calibration Files
7	1/14/2022 4:42:22 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1411.D
6	1/14/2022 5:14:49 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1412.D
5	1/14/2022 5:47:16 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1413.D
4	1/14/2022 6:19:44 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1414.D
3	1/14/2022 6:52:13 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1415.D
2	1/14/2022 7:24:38 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1416.D
1	1/14/2022 7:57:03 PM	\\MASSHUNTER\Org\Data\SV5975.I\sh011422\2 e8270c bna SIM\Jan1417.D
CCV	1/19/2022 3:46:05 AM	\\MASSHUNTER\Org\Data\SV5975.I\sh011822\1 e8270c bna SIM\Jan1824.D <=====

ISTD Compound:	Avg Resp	Mid Resp	CC Resp	Area%	A/M
1,4-Dichlorobenzene-d4	173591	173466	185938	107.19	M
Naphthalene-d8	313667	320346	338631	105.71	M
Acenaphthene-d10	169911	171827	186457	108.51	M
Phenanthrene-d10	347083	351005	381095	108.57	M
Chrysene-d12	256387	261208	260043	99.55	M
Perylene-d12	167073	172756	176150	101.97	M

Target Compound	AvgRF/R2	CC RF	Exp. Conc	Calc. Conc	%Dev	Area%	Curve Fit
1,4-Dichlorobenzene-d4	-----ISTD-----						
Nitrobenzene-d5	0.9999	0.6953	2.00	1.83	8.30	96.49	Quadratic
Naphthalene-d8	-----ISTD-----						
Naphthalene	1.3839	1.1533	2.00	1.67	-16.66	92.74	Avg RF
2-Methylnaphthalene	0.7724	0.7357	2.00	1.90	-4.75	101.37	Avg RF
1-Methylnaphthalene	0.8146	0.7509	2.00	1.84	-7.83	105.25	Avg RF
Acenaphthene-d10	-----ISTD-----						
2-Fluorobiphenyl	1.9227	1.8701	2.00	1.95	-2.73	110.18	Avg RF
Acenaphthylene	2.4514	2.2005	2.00	1.80	-10.23	102.55	Avg RF
Acenaphthene	1.5681	1.3357	2.00	1.70	-14.82	96.51	Avg RF
Fluorene	1.8554	1.7133	2.00	1.85	-7.66	104.06	Avg RF
Phenanthrene-d10	-----ISTD-----						
Phenanthrene	0.9999	1.1922	2.00	1.93	3.46	102.26	Quadratic
Anthracene	0.9999	1.0851	2.00	2.01	-0.65	107.13	Quadratic
o-Terphenyl	0.6510	0.5949	2.00	1.83	-8.62	101.37	Avg RF
Fluoranthene	1.3566	1.2194	2.00	1.80	-10.12	102.00	Avg RF
Chrysene-d12	-----ISTD-----						
Pyrene	2.0151	2.0206	2.00	2.01	0.27	100.67	Avg RF
Terphenyl-d14	0.9999	0.7585	2.00	2.06	-3.00	100.00	Quadratic
Benzo(a)Anthracene	0.9998	1.3485	2.00	2.12	-6.12	103.09	Quadratic
Chrysene	1.8307	1.6812	2.00	1.84	-8.17	95.81	Avg RF
Perylene-d12	-----ISTD-----						
Benzo(b)fluoranthene	1.8021	1.6504	2.00	1.83	-8.42	92.37	Avg RF
Benzo(k)fluoranthene	0.9995	2.0384	2.00	1.98	0.92	100.79	Quadratic
Benzo(a)pyrene	0.9999	1.4507	2.00	2.11	-5.56	106.93	Quadratic
Indeno(1,2,3-cd)pyrene	0.9998	1.3129	2.00	2.01	-0.31	99.35	Quadratic
Dibenzo(a,h)anthracene	1.5980	1.4548	2.00	1.82	-8.96	101.94	Avg RF
Benzo(g,h,i)perylene	0.9998	1.8549	2.00	1.95	2.53	97.97	Quadratic

A -- against Average; M -- against Mid Point; P -- against Previous CC in the Method;

Audit Trail report

Batch name and path: \\MASSHUNTER\Org\Data\SV5975.I\sh011822\1 e8270c bna SIM\QuantResults\011822 bna SIM1.batch.bin
Quant batch version: 10.0
Quant reporting version: 10.0

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdNewBatchTable	BL2000\jheine	1/18/2022 4:25:48 PM	Create new batch \\MASSHUNTER\Org\Data\SV5975.I\sh011822\1 e8270c bna SIM\011822 bna SIM1.batch.bin			✓	
CmdImportSamplesFromWorklist	BL2000\jheine	1/18/2022 4:25:54 PM	Add samples from worklist: \\MASSHUNTER\Org\Data\SV5975.I\sh011822\1 e8270c bna SIM\Jan1802.D, \\MASSHUNTER\Org\Data\SV5975.I\sh011822\1 e8270c bna SIM\Jan1801.D			✓	
CmdSetSampleAttribute	BL2000\jheine	1/18/2022 4:25:58 PM	Set SampleType = TuneCheck for sample Jan1801.D; previous value = Sample			✓	
CmdStartMethodEditing	BL2000\jheine	1/18/2022 4:26:52 PM	Start method editing			✓	
CmdImportMethodFromBatch	BL2000\jheine	1/18/2022 4:26:53 PM	Import method from batch \\MASSHUNTER\Org\Data\SV5975.I\sh011722\1 e8270c bna SIM\011722 bna SIM 1.batch.bin			✓	
CmdApplyMethodToAllSamples	BL2000\jheine	1/18/2022 4:26:57 PM	Apply method to all samples			✓	
CmdMethodClear	BL2000\jheine	1/18/2022 4:26:57 PM	Clear method			✓	
CmdEndMethodEditing	BL2000\jheine	1/18/2022 4:26:58 PM	End method editing			✓	
CmdQuantitate	BL2000\jheine	1/18/2022 4:27:01 PM	Quantitate all compounds in all samples			✓	
CmdSetSampleAttribute	BL2000\jheine	1/18/2022 4:27:03 PM	Set SampleType = CC for sample Jan1802.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/18/2022 4:27:06 PM	Set LevelName = CCV for sample Jan1802.D; previous value =			✓	
CmdQuantitate	BL2000\jheine	1/18/2022 4:27:09 PM	Quantitate all compounds in sample Jan1802.D			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/18/2022 4:27:29 PM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1802.D, from x, y = 5.928, 2503 to 6.066, 2080, result = -13848; previous integration is from x, y = 5.891, 80 to 6.140, 80 and previous response = 6674.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/18/2022 4:27:31 PM	Snap baseline for qualifier 102.0 of compound Naphthalene in sample Jan1802.D from x = 5.928 to x = 6.066, new integration is from x, y = 5.928, 2424 to 6.066, 100 and new response = -5363; previous integration is from x, y = 5.928, 2503 to 6.066, 2080 and previous response = -13848.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/18/2022 4:27:31 PM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1802.D to y = 100, new integration is from x, y = 5.928, 100 to 6.066, 100 and new response = 4216; previous integration is from x, y = 5.928, 2424 to 6.066, 100 and previous response = -5363.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/18/2022 4:27:44 PM	Manually integrate qualifier 153.0 of compound Acenaphthylene in sample Jan1802.D from x, y = 7.789, 1127 to 7.888, 2126; result = -6523			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/18/2022 4:27:45 PM	Snap baseline for qualifier 153.0 of compound Acenaphthylene in sample Jan1802.D from x = 7.789 to x = 7.888, new integration is from x, y = 7.789, 74 to 7.888, 127 and new response = 2608; previous integration is from x, y = 7.789, 1127 to 7.888, 2126 and previous response = -6523.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/18/2022 4:27:46 PM	Drop baseline for qualifier 153.0 of compound Acenaphthylene in sample Jan1802.D to y = 74, new integration is from x, y = 7.789, 74 to 7.888, 74 and new response = 2767; previous integration is from x, y = 7.789, 74 to 7.888, 127 and previous response = 2608.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/18/2022 4:27:54 PM	Manually integrate compound Acenaphthylene in sample Jan1802.D, from x, y = 7.789, 438 to 7.976, 991, result = 13436; previous integration is from x, y = 7.801, 100 to 7.913, 117 and previous response = 17843.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/18/2022 4:27:55 PM	Snap baseline for compound Acenaphthylene in sample Jan1802.D, from x = 7.789 to x = 7.976, new integration is from x, y = 7.789, 83 to 7.976, 129 and new response = 20257; previous integration is from x, y = 7.789, 438 to 7.976, 991 and previous response = 13436.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/18/2022 4:27:56 PM	Drop baseline for compound Acenaphthylene in sample Jan1802.D to y = 83, new integration is from x, y = 7.789, 83 to 7.976, 83 and new response = 20515; previous integration is from x, y = 7.789, 83 to 7.976, 129 and previous response = 20257.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/18/2022 4:27:57 PM	Set UserAnnotation = BA for compound Acenaphthylene in sample Jan1802.D; previous value =			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegratePeak	BL2000\jheine	1/18/2022 4:28:06 PM	Manually integrate compound Acenaphthene in sample Jan1802.D, from x, y = 8.013, 2390 to 8.125, 84, result = 3827; previous integration is from x, y = 7.976, 84 to 8.125, 84 and previous response = 12452.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/18/2022 4:28:07 PM	Drop baseline for compound Acenaphthene in sample Jan1802.D to y = 84, new integration is from x, y = 8.013, 84 to 8.125, 84 and new response = 11585; previous integration is from x, y = 8.013, 2390 to 8.125, 84 and previous response = 3827.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/18/2022 4:28:08 PM	Set UserAnnotation = CO for compound Acenaphthene in sample Jan1802.D; previous value =			✓	
CmdClearManualIntegration	BL2000\jheine	1/18/2022 4:28:10 PM	Clear manual integration of target signal for compound Acenaphthene in sample Jan1802.D			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/18/2022 4:28:11 PM	Set UserAnnotation = for compound Acenaphthene in sample Jan1802.D; previous value = CO			✓	
CmdSaveBatchTable	BL2000\jheine	1/18/2022 4:28:42 PM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh011822\1 e8270c bna SIM\QuantResults\011822 bna SIM1.batch.bin			✓	
CmdSaveBatchTable	BL2000\jheine	1/18/2022 4:28:49 PM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh011822\1 e8270c bna SIM\QuantResults\011822 bna SIM1.batch.bin			✓	
CmdSaveBatchTable	BL2000\jheine	1/18/2022 4:44:59 PM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh011822\1 e8270c bna SIM\QuantResults\011822 bna SIM1.batch.bin			✓	
CmdOpenBatchTable	BL2000\jheine	1/19/2022 8:24:25 AM	Open batch \\MASSHUNTER\Org\Data\SV5975.I\sh011822\1 e8270c bna SIM\011822 bna SIM1.batch.bin			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdImportSamplesFromWorklist	BL2000\jheine	1/19/2022 8:25:50 AM	Add samples from worklist: \\MASSHUNTER\Org\Data\SV5975.I\sh 011822\1 e8270c bna SIM\Jan1823.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011822\1 e8270c bna SIM\Jan1822.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011822\1 e8270c bna SIM\Jan1821.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011822\1 e8270c bna SIM\Jan1820.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011822\1 e8270c bna SIM\Jan1819.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011822\1 e8270c bna SIM\Jan1818.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011822\1 e8270c bna SIM\Jan1817.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011822\1 e8270c bna SIM\Jan1816.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011822\1 e8270c bna SIM\Jan1815.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011822\1 e8270c bna SIM\Jan1814.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011822\1 e8270c bna SIM\Jan1813.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011822\1 e8270c bna SIM\Jan1812.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011822\1 e8270c bna SIM\Jan1811.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011822\1 e8270c bna SIM\Jan1810.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011822\1 e8270c bna SIM\Jan1809.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011822\1 e8270c bna SIM\Jan1808.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011822\1 e8270c bna SIM\Jan1807.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011822\1 e8270c bna SIM\Jan1806.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011822\1 e8270c bna SIM\Jan1805.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011822\1 e8270c bna SIM\Jan1804.D, \\MASSHUNTER\Org\Data\SV5975.I\sh 011822\1 e8270c bna SIM\Jan1803.D			✓	
CmdImportSamplesFromWorklist	BL2000\jheine	1/19/2022 8:26:49 AM	Add samples from worklist: \\MASSHUNTER\Org\Data\SV5975.I\sh 011822\1 e8270c bna SIM\Jan1824.D			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:27:12 AM	Set SampleType = Matrix for sample Jan1806.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:27:15 AM	Set SampleType = MatrixDup for sample Jan1807.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:27:18 AM	Set SampleType = Matrix for sample Jan1808.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:27:21 AM	Set SampleType = MatrixDup for sample Jan1809.D; previous value = Sample			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:27:25 AM	Set SampleType = Blank for sample Jan1810.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:27:33 AM	Set SampleType = Matrix for sample Jan1815.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:27:37 AM	Set SampleType = Matrix for sample Jan1818.D; previous value = Sample			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:27:52 AM	Set MatrixSpikeGroup = 1.0 for sample Jan1808.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:27:52 AM	Set SampleInformation = MB-162889 for sample Jan1808.D; previous value =			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSetTargetCompoundAttribute	BL2000\jheine	1/19/2022 8:27:52 AM	Set ExpectedConcentration = SVOC-8270C-SIM-W-LLPAH for compound Nitrobenzene-d5 in sample Jan1808.D; previous value =				Agilent.MassSpectrometry.DataAnalysis.Quantitative.ApplicationCommandException: Input string was not in a correct format.Couldn't store <SVOC-8270C-SIM-W-LLPAH> in ExpectedConcentration Column. Expected type is Double. ---> System.ArgumentException: Input string was not in a correct format.Couldn't store <SVOC-8270C-SIM-W-LLPAH> in ExpectedConcentration Column. Expected type is Double. ---> System.FormatException: Input string was not in a correct format. at System.Number.ParseDouble(String value, NumberStyles options, NumberFormatInfo numfmt) at System.String.System.IConvertible.ToDouble(IFormatProvider provider) at System.Data.Common.DoubleStorage.Set(Int32 record, Object value) at System.Data.DataColumn.set_Item(Int32 record, Object value) --- End of inner exception stack trace --- at System.Data.DataColumn.set_Item(Int32 record, Object value) at System.Data.DataRow.set_Item(DataColumn column, Object value) at Agilent.MassSpectrometry.DataAnalysis.Quantitative.DataSetBase.SetColumnValue(RowIdBase rowId, String columnName, Object value) --- End of inner exception stack trace --- at Agilent.MassSpectrometry.DataAnalysis.Quantitative.DataSetBase.SetColumnValue(RowIdBase rowId, String columnName, Object value) at Agilent.MassSpectrometry.DataAnalysis.Quantitative.CmdSetTargetCompoundAttribute.Do() at Agilent.MassSpectrometry.CommandModel.CommandHistory.Invoke(ICommand cmd) at Agilent.MassSpectrometry.DataAnalysis.Quantitative.AppCommandContext._I

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
							nvoke(ICommand cmd)
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:28:05 AM	Set MatrixSpikeGroup = MB-162889 for sample Jan1808.D; previous value = 1.0			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:28:12 AM	Set SampleInformation = MatrixA for sample Jan1808.D; previous value = MB-162889			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:28:17 AM	Set MatrixSpikeGroup = MB-162889 for sample Jan1809.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:28:19 AM	Set MatrixSpikeGroup = MB-162889 for sample Jan1810.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:28:23 AM	Set MatrixSpikeGroup = B22010628-001C for sample Jan1814.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:28:25 AM	Set MatrixSpikeGroup = B22010628-001C for sample Jan1815.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:28:30 AM	Set MatrixSpikeGroup = B22010633-001C for sample Jan1817.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:28:31 AM	Set MatrixSpikeGroup = B22010633-001C for sample Jan1818.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:28:35 AM	Set SampleInformation = MatrixA for sample Jan1815.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:28:37 AM	Set SampleInformation = MatrixA for sample Jan1818.D; previous value =			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:28:39 AM	Set SampleInformation = MatrixA for sample Jan1809.D; previous value =			✓	
CmdQuantitate	BL2000\jheine	1/19/2022 8:28:52 AM	Quantitate all compounds in all samples			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/19/2022 8:29:58 AM	Manually integrate compound Benzo(a)pyrene in sample Jan1803.D, from x, y = 18.326, 102 to 18.400, 143, result = -230; previous integration is from x, y = 18.440, 61 to 18.623, 62 and previous response = 975.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/19/2022 8:29:59 AM	Snap baseline for compound Benzo(a)pyrene in sample Jan1803.D, from x = 18.326 to x = 18.400, new integration is from x, y = 18.326, 54 to 18.400, 59 and new response = 63; previous integration is from x, y = 18.326, 102 to 18.400, 143 and previous response = -230.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:30:00 AM	Drop baseline for compound Benzo(a)pyrene in sample Jan1803.D to y = 54, new integration is from x, y = 18.326, 54 to 18.400, 54 and new response = 74; previous integration is from x, y = 18.326, 54 to 18.400, 59 and previous response = 63.			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:30:04 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1803.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/19/2022 8:30:08 AM	Manually integrate compound Acenaphthene in sample Jan1803.D, from x, y = 8.013, 99 to 8.075, 64, result = 122; previous integration is from x, y = 7.967, 64 to 8.075, 64 and previous response = 1065.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:30:10 AM	Drop baseline for compound Acenaphthene in sample Jan1803.D to y = 64, new integration is from x, y = 8.013, 64 to 8.075, 64 and new response = 187; previous integration is from x, y = 8.013, 99 to 8.075, 64 and previous response = 122.			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:30:11 AM	Zero out primary peak of compound Acenaphthene in sample Jan1803.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/19/2022 8:30:16 AM	Manually integrate compound Chrysene in sample Jan1803.D, from x, y = 14.751, 77 to 14.838, 53, result = 132; previous integration is from x, y = 14.643, 53 to 14.838, 53 and previous response = 1402.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:30:17 AM	Drop baseline for compound Chrysene in sample Jan1803.D to y = 53, new integration is from x, y = 14.751, 53 to 14.838, 53 and new response = 194; previous integration is from x, y = 14.751, 77 to 14.838, 53 and previous response = 132.			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:30:19 AM	Zero out primary peak of compound Chrysene in sample Jan1803.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/19/2022 8:30:25 AM	Manually integrate compound Benzo(a)Anthracene in sample Jan1803.D, from x, y = 14.643, 53 to 14.751, 81, result = 1118; previous integration is from x, y = 14.643, 53 to 14.838, 53 and previous response = 1402.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:30:26 AM	Drop baseline for compound Benzo(a)Anthracene in sample Jan1803.D to y = 53, new integration is from x, y = 14.643, 53 to 14.751, 53 and new response = 1208; previous integration is from x, y = 14.643, 53 to 14.751, 81 and previous response = 1118.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:30:28 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1803.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/19/2022 8:30:46 AM	Manually integrate compound Fluorene in sample Jan1804.D, from x, y = 8.649, 65 to 8.698, 66, result = 39; previous integration is from x, y = 8.936, 62 to 9.110, 62 and previous response = 7763.			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:30:47 AM	Zero out primary peak of compound Fluorene in sample Jan1804.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:30:50 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1804.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:30:53 AM	Zero out primary peak of compound Acenaphthene in sample Jan1804.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:30:55 AM	Zero out primary peak of compound Chrysene in sample Jan1804.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:30:57 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1804.D			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/19/2022 8:31:16 AM	Snap baseline for qualifier 115.0 of compound 2-Methylnaphthalene in sample Jan1805.D from x = 6.753 to x = 6.815, new integration is from x, y = 6.753, 3235 to 6.815, 1879 and new response = 35785; previous integration is from x, y = 6.753, 217 to 6.815, 219 and previous response = 44547.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:31:17 AM	Drop baseline for qualifier 115.0 of compound 2-Methylnaphthalene in sample Jan1805.D to y = 1879, new integration is from x, y = 6.753, 1879 to 6.815, 1879 and new response = 38325; previous integration is from x, y = 6.753, 3235 to 6.815, 1879 and previous response = 35785.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/19/2022 8:31:29 AM	Manually integrate qualifier 115.0 of compound 1-Methylnaphthalene in sample Jan1805.D, from x, y = 6.865, 2668 to 6.915, 3582, result = 22867; previous integration is from x, y = 6.815, 219 to 6.915, 220 and previous response = 38492.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:31:31 AM	Drop baseline for qualifier 115.0 of compound 1-Methylnaphthalene in sample Jan1805.D to y = 2668, new integration is from x, y = 6.865, 2668 to 6.915, 2668 and new response = 24237; previous integration is from x, y = 6.865, 2668 to 6.915, 3582 and previous response = 22867.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:31:41 AM	Zero out qualifier peak of compound Nitrobenzene-d5 128.0 in sample Jan1805.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:31:42 AM	Zero out primary peak of compound Nitrobenzene-d5 in sample Jan1805.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/19/2022 8:31:50 AM	Manually integrate compound Naphthalene in sample Jan1805.D, from x, y = 5.928, 498 to 5.991, 107, result = 16429; previous integration is from x, y = 5.891, 107 to 5.991, 107 and previous response = 18738.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:31:51 AM	Drop baseline for compound Naphthalene in sample Jan1805.D to y = 107, new integration is from x, y = 5.928, 107 to 5.991, 107 and new response = 17159; previous integration is from x, y = 5.928, 498 to 5.991, 107 and previous response = 16429.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/19/2022 8:31:56 AM	Manually integrate qualifier 129.0 of compound Naphthalene in sample Jan1805.D, from x, y = 5.928, 348 to 5.966, 367, result = 6071; previous integration is from x, y = 5.907, 527 to 5.966, 592 and previous response = 6026.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/19/2022 8:32:03 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1805.D, from x, y = 5.928, 582 to 5.991, 300, result = 4071; previous integration is from x, y = 5.904, 439 to 5.985, 439 and previous response = 5647.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:32:04 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1805.D to y = 300, new integration is from x, y = 5.928, 300 to 5.991, 300 and new response = 4598; previous integration is from x, y = 5.928, 582 to 5.991, 300 and previous response = 4071.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/19/2022 8:32:20 AM	Manually integrate compound Benzo(a)pyrene in sample Jan1805.D, from x, y = 18.339, 54 to 18.413, 59, result = 62; previous integration is from x, y = 18.440, 62 to 18.598, 63 and previous response = 912.			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:32:21 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1805.D			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/19/2022 8:32:28 AM	Manually integrate qualifier 167.0 of compound Fluorene in sample Jan1805.D from x, y = 8.674, 164 to 8.698, 162; result = 324			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/19/2022 8:32:32 AM	Manually integrate qualifier 167.0 of compound Fluorene in sample Jan1805.D, from x, y = 8.661, 154 to 8.698, 162, result = 544; previous integration is from x, y = 8.674, 164 to 8.698, 162 and previous response = 324.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:32:33 AM	Drop baseline for qualifier 167.0 of compound Fluorene in sample Jan1805.D to y = 154, new integration is from x, y = 8.661, 154 to 8.698, 154 and new response = 553; previous integration is from x, y = 8.661, 154 to 8.698, 162 and previous response = 544.			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:32:36 AM	Zero out primary peak of compound Fluorene in sample Jan1805.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:32:41 AM	Zero out primary peak of compound Acenaphthylene in sample Jan1805.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:32:43 AM	Zero out primary peak of compound Chrysene in sample Jan1805.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:32:45 AM	Zero out primary peak of compound Acenaphthene in sample Jan1805.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:32:45 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1805.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/19/2022 8:33:08 AM	Manually integrate compound Acenaphthene in sample Jan1806.D, from x, y = 8.013, 118 to 8.125, 63, result = 1269; previous integration is from x, y = 7.965, 63 to 8.125, 63 and previous response = 2332.			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	1/19/2022 8:33:12 AM	Split peak for compound Acenaphthene in sample Jan1806.D and keep right peak, new integration is from x, y = 8.013, 118.079422382671 to 8.125, 63.3442307692308 and new response = 1269, previous integration is from x, y = 8.013, 118 to 8.125, 63 and previous response = 1269.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:33:14 AM	Drop baseline for compound Acenaphthene in sample Jan1806.D to y = 63, new integration is from x, y = 8.013, 63 to 8.125, 63 and new response = 1454; previous integration is from x, y = 8.013, 118 to 8.125, 63 and previous response = 1269.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/19/2022 8:33:16 AM	Set UserAnnotation = CO for compound Acenaphthene in sample Jan1806.D; previous value =			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/19/2022 8:33:27 AM	Set UserAnnotation = CO for compound Naphthalene in sample Jan1805.D; previous value =			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/19/2022 8:33:58 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1807.D, from x, y = 5.928, 281 to 6.028, 86, result = 5052; previous integration is from x, y = 5.891, 84 to 6.028, 86 and previous response = 7917.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:34:00 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1807.D to y = 86, new integration is from x, y = 5.928, 86 to 6.028, 86 and new response = 5637; previous integration is from x, y = 5.928, 281 to 6.028, 86 and previous response = 5052.			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	1/19/2022 8:34:28 AM	Split peak for compound Acenaphthene in sample Jan1807.D and keep right peak, new integration is from x, y = 7.975, 71.2303022139263 to 8.125, 75.7191940961966 and new response = 22319, previous integration is from x, y = 7.975, 71 to 8.125, 76 and previous response = 22319.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/19/2022 8:35:06 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1808.D, from x, y = 5.928, 666 to 6.028, 82, result = 4628; previous integration is from x, y = 5.903, 83 to 6.028, 82 and previous response = 8563.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:35:08 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1808.D to y = 82, new integration is from x, y = 5.928, 82 to 6.028, 82 and new response = 6378; previous integration is from x, y = 5.928, 666 to 6.028, 82 and previous response = 4628.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/19/2022 8:38:23 AM	Manually integrate compound Benzo(g,h,i)perylene in sample Jan1808.D, from x, y = 20.501, 3122 to 20.611, 884, result = 29700; previous integration is from x, y = 20.509, 1089 to 20.611, 884 and previous response = 36436.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/19/2022 8:38:26 AM	Manually integrate compound Benzo(g,h,i)perylene in sample Jan1808.D, from x, y = 20.501, 3122 to 20.674, 1129, result = 23071; previous integration is from x, y = 20.501, 3122 to 20.611, 884 and previous response = 29700.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/19/2022 8:38:27 AM	Snap baseline for compound Benzo(g,h,i)perylene in sample Jan1808.D, from x = 20.501 to x = 20.674, new integration is from x, y = 20.501, 171 to 20.674, 420 and new response = 42065; previous integration is from x, y = 20.501, 3122 to 20.674, 1129 and previous response = 23071.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:38:28 AM	Drop baseline for compound Benzo(g,h,i)perylene in sample Jan1808.D to y = 171, new integration is from x, y = 20.501, 171 to 20.674, 171 and new response = 43357; previous integration is from x, y = 20.501, 171 to 20.674, 420 and previous response = 42065.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/19/2022 8:38:29 AM	Set UserAnnotation = BA for compound Benzo(g,h,i)perylene in sample Jan1808.D; previous value =			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/19/2022 8:39:20 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1809.D, from x, y = 5.928, 604 to 6.028, 79, result = 3747; previous integration is from x, y = 5.903, 79 to 6.028, 79 and previous response = 7500.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:39:22 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1809.D to y = 79, new integration is from x, y = 5.928, 79 to 6.028, 79 and new response = 5319; previous integration is from x, y = 5.928, 604 to 6.028, 79 and previous response = 3747.			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:40:28 AM	Zero out primary peak of compound Fluorene in sample Jan1810.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:40:30 AM	Zero out primary peak of compound Fluorene in sample Jan1810.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/19/2022 8:40:36 AM	Manually integrate compound Benzo(a)pyrene in sample Jan1810.D, from x, y = 18.326, 55 to 18.401, 63, result = 67; previous integration is from x, y = 18.425, 57 to 18.598, 58 and previous response = 946.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:40:37 AM	Drop baseline for compound Benzo(a)pyrene in sample Jan1810.D to y = 55, new integration is from x, y = 18.326, 55 to 18.401, 55 and new response = 85; previous integration is from x, y = 18.326, 55 to 18.401, 63 and previous response = 67.			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:40:39 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1810.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:40:44 AM	Zero out primary peak of compound Acenaphthene in sample Jan1810.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/19/2022 8:40:50 AM	Manually integrate compound Chrysene in sample Jan1810.D, from x, y = 14.751, 146 to 14.839, 144, result = -224; previous integration is from x, y = 14.642, 53 to 14.751, 53 and previous response = 1232.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/19/2022 8:40:51 AM	Snap baseline for compound Chrysene in sample Jan1810.D, from x = 14.751 to x = 14.839, new integration is from x, y = 14.751, 104 to 14.839, 62 and new response = 99; previous integration is from x, y = 14.751, 146 to 14.839, 144 and previous response = -224.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:40:52 AM	Drop baseline for compound Chrysene in sample Jan1810.D to y = 62, new integration is from x, y = 14.751, 62 to 14.839, 62 and new response = 208; previous integration is from x, y = 14.751, 104 to 14.839, 62 and previous response = 99.			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:40:54 AM	Zero out primary peak of compound Chrysene in sample Jan1810.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:40:58 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1810.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:41:10 AM	Zero out primary peak of compound Fluorene in sample Jan1811.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:41:12 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1811.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:41:15 AM	Zero out primary peak of compound Acenaphthene in sample Jan1811.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/19/2022 8:41:20 AM	Manually integrate compound Chrysene in sample Jan1811.D, from x, y = 14.751, 71 to 14.838, 53, result = 92; previous integration is from x, y = 14.642, 52 to 14.838, 53 and previous response = 1341.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:41:22 AM	Drop baseline for compound Chrysene in sample Jan1811.D to y = 53, new integration is from x, y = 14.751, 53 to 14.838, 53 and new response = 139; previous integration is from x, y = 14.751, 71 to 14.838, 53 and previous response = 92.			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:41:23 AM	Zero out primary peak of compound Chrysene in sample Jan1811.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:41:27 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1811.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:41:36 AM	Zero out primary peak of compound Fluorene in sample Jan1812.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:41:38 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1812.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/19/2022 8:41:48 AM	Manually integrate compound Acenaphthene in sample Jan1812.D, from x, y = 8.025, 86 to 8.088, 65, result = 48; previous integration is from x, y = 7.976, 65 to 8.088, 65 and previous response = 1009.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:41:50 AM	Drop baseline for compound Acenaphthene in sample Jan1812.D to y = 65, new integration is from x, y = 8.025, 65 to 8.088, 65 and new response = 87; previous integration is from x, y = 8.025, 86 to 8.088, 65 and previous response = 48.			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:41:51 AM	Zero out primary peak of compound Acenaphthene in sample Jan1812.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:41:55 AM	Zero out primary peak of compound Chrysene in sample Jan1812.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:41:56 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1812.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:42:27 AM	Zero out primary peak of compound Fluorene in sample Jan1813.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:42:32 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1813.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:42:46 AM	Zero out primary peak of compound Acenaphthene in sample Jan1813.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/19/2022 8:42:52 AM	Manually integrate compound Chrysene in sample Jan1813.D, from x, y = 14.751, 81 to 14.851, 53, result = 27; previous integration is from x, y = 14.641, 52 to 14.851, 53 and previous response = 1275.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:42:54 AM	Drop baseline for compound Chrysene in sample Jan1813.D to y = 53, new integration is from x, y = 14.751, 53 to 14.851, 53 and new response = 111; previous integration is from x, y = 14.751, 81 to 14.851, 53 and previous response = 27.			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:42:56 AM	Zero out primary peak of compound Chrysene in sample Jan1813.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:43:06 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1813.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:43:24 AM	Zero out primary peak of compound Fluorene in sample Jan1814.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:43:27 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1814.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:43:29 AM	Zero out primary peak of compound Acenaphthene in sample Jan1814.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:43:35 AM	Zero out primary peak of compound Chrysene in sample Jan1814.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:43:37 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1814.D			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/19/2022 8:43:54 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1815.D, from x, y = 5.928, 643 to 6.028, 75, result = 4920; previous integration is from x, y = 5.891, 75 to 6.028, 75 and previous response = 8835.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:43:56 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1815.D to y = 75, new integration is from x, y = 5.928, 75 to 6.028, 75 and new response = 6623; previous integration is from x, y = 5.928, 643 to 6.028, 75 and previous response = 4920.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/19/2022 8:44:07 AM	Manually integrate compound 1-Methylnaphthalene in sample Jan1815.D, from x, y = 6.865, 2302 to 6.952, 3279, result = 7379; previous integration is from x, y = 6.752, 72 to 6.865, 72 and previous response = 25530.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/19/2022 8:44:08 AM	Snap baseline for compound 1-Methylnaphthalene in sample Jan1815.D, from x = 6.865 to x = 6.952, new integration is from x, y = 6.865, 329 to 6.952, 393 and new response = 20121; previous integration is from x, y = 6.865, 2302 to 6.952, 3279 and previous response = 7379.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:44:09 AM	Drop baseline for compound 1-Methylnaphthalene in sample Jan1815.D to y = 329, new integration is from x, y = 6.865, 329 to 6.952, 329 and new response = 20289; previous integration is from x, y = 6.865, 329 to 6.952, 393 and previous response = 20121.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/19/2022 8:44:20 AM	Manually integrate qualifier 153.0 of compound Acenaphthylene in sample Jan1815.D from x, y = 7.801, 962 to 7.863, 2877; result = -1577			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/19/2022 8:44:21 AM	Snap baseline for qualifier 153.0 of compound Acenaphthylene in sample Jan1815.D from x = 7.801 to x = 7.863, new integration is from x, y = 7.801, 62 to 7.863, 250 and new response = 5017; previous integration is from x, y = 7.801, 962 to 7.863, 2877 and previous response = -1577.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:44:22 AM	Drop baseline for qualifier 153.0 of compound Acenaphthylene in sample Jan1815.D to y = 62, new integration is from x, y = 7.801, 62 to 7.863, 62 and new response = 5369; previous integration is from x, y = 7.801, 62 to 7.863, 250 and previous response = 5017.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/19/2022 8:44:34 AM	Manually integrate qualifier 176.0 of compound Phenanthrene in sample Jan1815.D from x, y = 9.745, 56 to 9.830, 1810; result = 6001			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:44:35 AM	Drop baseline for qualifier 176.0 of compound Phenanthrene in sample Jan1815.D to y = 56, new integration is from x, y = 9.745, 56 to 9.830, 56 and new response = 10428; previous integration is from x, y = 9.745, 56 to 9.830, 1810 and previous response = 6001.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/19/2022 8:44:42 AM	Manually integrate qualifier 176.0 of compound Anthracene in sample Jan1815.D, from x, y = 9.830, 2794 to 9.928, 56, result = 1108; previous integration is from x, y = 9.745, 56 to 9.928, 56 and previous response = 19652.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:44:44 AM	Drop baseline for qualifier 176.0 of compound Anthracene in sample Jan1815.D to y = 56, new integration is from x, y = 9.830, 56 to 9.928, 56 and new response = 9225; previous integration is from x, y = 9.830, 2794 to 9.928, 56 and previous response = 1108.			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:45:26 AM	Zero out primary peak of compound Fluorene in sample Jan1816.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:45:28 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1816.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:45:30 AM	Zero out primary peak of compound Acenaphthene in sample Jan1816.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:45:32 AM	Zero out primary peak of compound Chrysene in sample Jan1816.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:45:34 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1816.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:46:09 AM	Zero out primary peak of compound Fluorene in sample Jan1817.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/19/2022 8:46:15 AM	Manually integrate compound Benzo(a)pyrene in sample Jan1817.D, from x, y = 18.339, 73 to 18.388, 151, result = -124; previous integration is from x, y = 18.438, 57 to 18.611, 58 and previous response = 1008.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/19/2022 8:46:16 AM	Snap baseline for compound Benzo(a)pyrene in sample Jan1817.D, from x = 18.339 to x = 18.388, new integration is from x, y = 18.339, 54 to 18.388, 58 and new response = 42; previous integration is from x, y = 18.339, 73 to 18.388, 151 and previous response = -124.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:46:17 AM	Drop baseline for compound Benzo(a)pyrene in sample Jan1817.D to y = 54, new integration is from x, y = 18.339, 54 to 18.388, 54 and new response = 48; previous integration is from x, y = 18.339, 54 to 18.388, 58 and previous response = 42.			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:46:19 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1817.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/19/2022 8:46:25 AM	Manually integrate compound Acenaphthene in sample Jan1817.D, from x, y = 8.013, 97 to 8.063, 66, result = 84; previous integration is from x, y = 7.976, 67 to 8.063, 66 and previous response = 972.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:46:26 AM	Drop baseline for compound Acenaphthene in sample Jan1817.D to y = 66, new integration is from x, y = 8.013, 66 to 8.063, 66 and new response = 130; previous integration is from x, y = 8.013, 97 to 8.063, 66 and previous response = 84.			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:46:27 AM	Zero out primary peak of compound Acenaphthene in sample Jan1817.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/19/2022 8:46:33 AM	Manually integrate compound Chrysene in sample Jan1817.D, from x, y = 14.739, 184 to 14.863, 168, result = -463; previous integration is from x, y = 14.623, 51 to 14.739, 51 and previous response = 1498.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/19/2022 8:46:34 AM	Snap baseline for compound Chrysene in sample Jan1817.D, from x = 14.739 to x = 14.863, new integration is from x, y = 14.739, 109 to 14.863, 60 and new response = 219; previous integration is from x, y = 14.739, 184 to 14.863, 168 and previous response = -463.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:46:35 AM	Drop baseline for compound Chrysene in sample Jan1817.D to y = 60, new integration is from x, y = 14.739, 60 to 14.863, 60 and new response = 402; previous integration is from x, y = 14.739, 109 to 14.863, 60 and previous response = 219.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/19/2022 8:46:41 AM	Manually integrate qualifier 229.0 of compound Chrysene in sample Jan1817.D from x, y = 14.751, 63 to 14.826, 51; result = 94			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:46:42 AM	Drop baseline for qualifier 229.0 of compound Chrysene in sample Jan1817.D to y = 51, new integration is from x, y = 14.751, 51 to 14.826, 51 and new response = 120; previous integration is from x, y = 14.751, 63 to 14.826, 51 and previous response = 94.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/19/2022 8:46:45 AM	Manually integrate qualifier 226.0 of compound Chrysene in sample Jan1817.D, from x, y = 14.739, 51 to 14.863, 70, result = 100; previous integration is from x, y = 14.739, 51 to 14.963, 51 and previous response = 202.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/19/2022 8:46:47 AM	Snap baseline for qualifier 226.0 of compound Chrysene in sample Jan1817.D from x = 14.739 to x = 14.863, new integration is from x, y = 14.739, 66 to 14.863, 56 and new response = 97; previous integration is from x, y = 14.739, 51 to 14.863, 70 and previous response = 100.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:46:50 AM	Drop baseline for qualifier 226.0 of compound Chrysene in sample Jan1817.D to y = 56, new integration is from x, y = 14.739, 56 to 14.863, 56 and new response = 134; previous integration is from x, y = 14.739, 66 to 14.863, 56 and previous response = 97.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/19/2022 8:47:24 AM	Snap baseline for qualifier 229.0 of compound Chrysene in sample Jan1817.D from x = 14.751 to x = 14.826, new integration is from x, y = 14.751, 82 to 14.826, 61 and new response = 29; previous integration is from x, y = 14.751, 51 to 14.826, 51 and previous response = 120.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrate DropBaseline	BL2000\jheine	1/19/2022 8:47:25 AM	Drop baseline for qualifier 229.0 of compound Chrysene in sample Jan1817.D to y = 61, new integration is from x, y = 14.751, 61 to 14.826, 61 and new response = 76; previous integration is from x, y = 14.751, 82 to 14.826, 61 and previous response = 29.			✓	
CmdManuallyIntegrate QualifierPeak	BL2000\jheine	1/19/2022 8:47:40 AM	Manually integrate qualifier 101.0 of compound Pyrene in sample Jan1817.D, from x, y = 11.751, 62 to 11.818, 65, result = 110; previous integration is from x, y = 11.751, 62 to 11.930, 63 and previous response = 171.			✓	
CmdManuallyIntegrate DropBaseline	BL2000\jheine	1/19/2022 8:47:41 AM	Drop baseline for qualifier 101.0 of compound Pyrene in sample Jan1817.D to y = 62, new integration is from x, y = 11.751, 62 to 11.818, 62 and new response = 117; previous integration is from x, y = 11.751, 62 to 11.818, 65 and previous response = 110.			✓	
CmdManuallyIntegrate QualifierPeak	BL2000\jheine	1/19/2022 8:47:51 AM	Manually integrate qualifier 101.0 of compound Fluoranthene in sample Jan1817.D from x, y = 11.374, 59 to 11.473, 58; result = 86			✓	
CmdManuallyIntegrate DropBaseline	BL2000\jheine	1/19/2022 8:47:52 AM	Drop baseline for qualifier 101.0 of compound Fluoranthene in sample Jan1817.D to y = 58, new integration is from x, y = 11.374, 58 to 11.473, 58 and new response = 89; previous integration is from x, y = 11.374, 59 to 11.473, 58 and previous response = 86.			✓	
CmdManuallyIntegrate QualifierPeak	BL2000\jheine	1/19/2022 8:47:58 AM	Manually integrate qualifier 229.0 of compound Benzo(a)Anthracene in sample Jan1817.D, from x, y = 14.627, 51 to 14.751, 76, result = 512; previous integration is from x, y = 14.627, 51 to 14.826, 51 and previous response = 726.			✓	
CmdManuallyIntegrate DropBaseline	BL2000\jheine	1/19/2022 8:48:00 AM	Drop baseline for qualifier 229.0 of compound Benzo(a)Anthracene in sample Jan1817.D to y = 51, new integration is from x, y = 14.627, 51 to 14.751, 51 and new response = 605; previous integration is from x, y = 14.627, 51 to 14.751, 76 and previous response = 512.			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:48:28 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1817.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/19/2022 8:48:43 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1818.D, from x, y = 5.928, 663 to 6.028, 74, result = 4043; previous integration is from x, y = 5.903, 74 to 6.028, 74 and previous response = 8113.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:48:44 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1818.D to y = 74, new integration is from x, y = 5.928, 74 to 6.028, 74 and new response = 5811; previous integration is from x, y = 5.928, 663 to 6.028, 74 and previous response = 4043.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/19/2022 8:48:56 AM	Manually integrate qualifier 153.0 of compound Acenaphthylene in sample Jan1818.D from x, y = 7.789, 2375 to 7.876, 3507; result = -10050			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/19/2022 8:48:58 AM	Snap baseline for qualifier 153.0 of compound Acenaphthylene in sample Jan1818.D from x = 7.789 to x = 7.876, new integration is from x, y = 7.789, 63 to 7.876, 179 and new response = 4710; previous integration is from x, y = 7.789, 2375 to 7.876, 3507 and previous response = -10050.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:48:58 AM	Drop baseline for qualifier 153.0 of compound Acenaphthylene in sample Jan1818.D to y = 63, new integration is from x, y = 7.789, 63 to 7.876, 63 and new response = 5014; previous integration is from x, y = 7.789, 63 to 7.876, 179 and previous response = 4710.			✓	
CmdManuallyIntegrateSplit	BL2000\jheine	1/19/2022 8:49:09 AM	Split qualifier 176.0 of compound Phenanthrene in sample Jan1818.D and keep left peak, new integration is from x, y = 9.750, 57.2954931972789 to 9.830, 57.2954931972789 and new response = 10008, previous integration is from x, y = 9.750, 57 to 9.879, 57 and previous response = 18207.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/19/2022 8:49:24 AM	Manually integrate qualifier 176.0 of compound Anthracene in sample Jan1818.D from x, y = 9.830, 731 to 9.916, 1093; result = 4371			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/19/2022 8:49:26 AM	Snap baseline for qualifier 176.0 of compound Anthracene in sample Jan1818.D from x = 9.830 to x = 9.916, new integration is from x, y = 9.830, 243 to 9.916, 202 and new response = 7949; previous integration is from x, y = 9.830, 731 to 9.916, 1093 and previous response = 4371.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:49:26 AM	Drop baseline for qualifier 176.0 of compound Anthracene in sample Jan1818.D to y = 202, new integration is from x, y = 9.830, 202 to 9.916, 202 and new response = 8056; previous integration is from x, y = 9.830, 243 to 9.916, 202 and previous response = 7949.			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:50:43 AM	Zero out primary peak of compound Fluorene in sample Jan1819.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:50:46 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1819.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:50:49 AM	Zero out primary peak of compound Acenaphthene in sample Jan1819.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:50:51 AM	Zero out primary peak of compound Chrysene in sample Jan1819.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:50:53 AM	Zero out primary peak of compound o-Terphenyl in sample Jan1819.D			✓	
CmdClearManualIntegration	BL2000\jheine	1/19/2022 8:50:58 AM	Clear manual integration of target signal for compound o-Terphenyl in sample Jan1819.D			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/19/2022 8:51:05 AM	Manually integrate qualifier 215.0 of compound o-Terphenyl in sample Jan1819.D from x, y = 10.274, 54 to 10.324, 54; result = 135			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:51:15 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1819.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:51:28 AM	Zero out primary peak of compound Fluorene in sample Jan1820.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:51:31 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1820.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:51:33 AM	Zero out primary peak of compound Acenaphthene in sample Jan1820.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:51:36 AM	Zero out primary peak of compound Chrysene in sample Jan1820.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:51:38 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1820.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:51:57 AM	Zero out primary peak of compound Fluorene in sample Jan1821.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:51:59 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1821.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:52:03 AM	Zero out primary peak of compound Acenaphthene in sample Jan1821.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:52:07 AM	Zero out primary peak of compound Chrysene in sample Jan1821.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:52:08 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1821.D			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:52:16 AM	Zero out primary peak of compound Fluorene in sample Jan1822.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:52:19 AM	Zero out primary peak of compound Benzo(a)pyrene in sample Jan1822.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:52:24 AM	Zero out primary peak of compound Acenaphthene in sample Jan1822.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:52:27 AM	Zero out primary peak of compound Chrysene in sample Jan1822.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:52:29 AM	Zero out primary peak of compound Benzo(a)Anthracene in sample Jan1822.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:52:42 AM	Zero out primary peak of compound Fluorene in sample Jan1823.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/19/2022 8:53:12 AM	Manually integrate compound Benzo(b)fluoranthene in sample Jan1823.D, from x, y = 17.671, 62 to 17.758, 122, result = 1571; previous integration is from x, y = 17.690, 189 to 17.758, 207 and previous response = 1116.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:53:14 AM	Drop baseline for compound Benzo(b)fluoranthene in sample Jan1823.D to y = 62, new integration is from x, y = 17.671, 62 to 17.758, 62 and new response = 1726; previous integration is from x, y = 17.671, 62 to 17.758, 122 and previous response = 1571.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/19/2022 8:53:18 AM	Manually integrate qualifier 253.0 of compound Benzo(b)fluoranthene in sample Jan1823.D, from x, y = 17.673, 76 to 17.758, 97, result = 347; previous integration is from x, y = 17.673, 76 to 17.857, 78 and previous response = 593.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:53:20 AM	Drop baseline for qualifier 253.0 of compound Benzo(b)fluoranthene in sample Jan1823.D to y = 76, new integration is from x, y = 17.673, 76 to 17.758, 76 and new response = 402; previous integration is from x, y = 17.673, 76 to 17.758, 97 and previous response = 347.			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/19/2022 8:53:30 AM	Manually integrate compound Indeno(1,2,3-cd)pyrene in sample Jan1823.D, from x, y = 20.167, 68 to 20.254, 163, result = 453; previous integration is from x, y = 20.167, 68 to 20.357, 71 and previous response = 812.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:53:31 AM	Drop baseline for compound Indeno(1,2,3-cd)pyrene in sample Jan1823.D to y = 68, new integration is from x, y = 20.167, 68 to 20.254, 68 and new response = 697; previous integration is from x, y = 20.167, 68 to 20.254, 163 and previous response = 453.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/19/2022 8:53:36 AM	Manually integrate qualifier 138.0 of compound Indeno(1,2,3-cd)pyrene in sample Jan1823.D, from x, y = 20.173, 106 to 20.254, 135, result = 137; previous integration is from x, y = 20.173, 106 to 20.293, 107 and previous response = 234.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:53:37 AM	Drop baseline for qualifier 138.0 of compound Indeno(1,2,3-cd)pyrene in sample Jan1823.D to y = 106, new integration is from x, y = 20.173, 106 to 20.254, 106 and new response = 209; previous integration is from x, y = 20.173, 106 to 20.254, 135 and previous response = 137.			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/19/2022 8:53:40 AM	Set UserAnnotation = CO for compound Indeno(1,2,3-cd)pyrene in sample Jan1823.D; previous value =			✓	
CmdSetTargetCompoundAttribute	BL2000\jheine	1/19/2022 8:53:44 AM	Set UserAnnotation = BA for compound Benzo(b)fluoranthene in sample Jan1823.D; previous value =			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:53:50 AM	Zero out primary peak of compound Acenaphthylene in sample Jan1823.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:53:54 AM	Zero out primary peak of compound Acenaphthene in sample Jan1823.D			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/19/2022 8:54:04 AM	Manually integrate qualifier 253.0 of compound Benzo(k)fluoranthene in sample Jan1823.D from x, y = 17.758, 137 to 17.820, 105; result = 15			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/19/2022 8:54:06 AM	Snap baseline for qualifier 253.0 of compound Benzo(k)fluoranthene in sample Jan1823.D from x = 17.758 to x = 17.820, new integration is from x, y = 17.758, 125 to 17.820, 81 and new response = 83; previous integration is from x, y = 17.758, 137 to 17.820, 105 and previous response = 15.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:54:07 AM	Drop baseline for qualifier 253.0 of compound Benzo(k)fluoranthene in sample Jan1823.D to y = 81, new integration is from x, y = 17.758, 81 to 17.820, 81 and new response = 165; previous integration is from x, y = 17.758, 125 to 17.820, 81 and previous response = 83.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:54:15 AM	Zero out primary peak of compound Dibenzo(a,h)anthracene in sample Jan1823.D			✓	
CmdManuallyIntegratePeak	BL2000\jheine	1/19/2022 8:54:22 AM	Manually integrate compound Anthracene in sample Jan1823.D, from x, y = 9.830, 224 to 9.891, 248, result = 71; previous integration is from x, y = 9.744, 185 to 9.821, 183 and previous response = 815.			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/19/2022 8:54:23 AM	Snap baseline for compound Anthracene in sample Jan1823.D, from x = 9.830 to x = 9.891, new integration is from x, y = 9.830, 173 to 9.891, 184 and new response = 284; previous integration is from x, y = 9.830, 224 to 9.891, 248 and previous response = 71.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:54:24 AM	Drop baseline for compound Anthracene in sample Jan1823.D to y = 173, new integration is from x, y = 9.830, 173 to 9.891, 173 and new response = 304; previous integration is from x, y = 9.830, 173 to 9.891, 184 and previous response = 284.			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:54:26 AM	Zero out primary peak of compound Anthracene in sample Jan1823.D			✓	
CmdZeroOutPeak	BL2000\jheine	1/19/2022 8:54:31 AM	Zero out primary peak of compound Phenanthrene in sample Jan1823.D			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/19/2022 8:55:00 AM	Manually integrate qualifier 102.0 of compound Naphthalene in sample Jan1824.D, from x, y = 5.928, 545 to 6.016, 87, result = 2632; previous integration is from x, y = 5.894, 79 to 6.016, 87 and previous response = 5989.			✓	
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:55:01 AM	Drop baseline for qualifier 102.0 of compound Naphthalene in sample Jan1824.D to y = 87, new integration is from x, y = 5.928, 87 to 6.016, 87 and new response = 3832; previous integration is from x, y = 5.928, 545 to 6.016, 87 and previous response = 2632.			✓	
CmdManuallyIntegrateQualifierPeak	BL2000\jheine	1/19/2022 8:55:13 AM	Manually integrate qualifier 153.0 of compound Acenaphthylene in sample Jan1824.D from x, y = 7.801, 1068 to 7.863, 1417; result = -1994			✓	
CmdManuallyIntegrateSnapBaseline	BL2000\jheine	1/19/2022 8:55:15 AM	Snap baseline for qualifier 153.0 of compound Acenaphthylene in sample Jan1824.D from x = 7.801 to x = 7.863, new integration is from x, y = 7.801, 64 to 7.863, 172 and new response = 2211; previous integration is from x, y = 7.801, 1068 to 7.863, 1417 and previous response = -1994.			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdManuallyIntegrateDropBaseline	BL2000\jheine	1/19/2022 8:55:16 AM	Drop baseline for qualifier 153.0 of compound Acenaphthylene in sample Jan1824.D to y = 64, new integration is from x, y = 7.801, 64 to 7.863, 64 and new response = 2413; previous integration is from x, y = 7.801, 64 to 7.863, 172 and previous response = 2211.			✓	
CmdSaveBatchTable	BL2000\jheine	1/19/2022 8:56:20 AM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh011822\1 e8270c bna SIM\QuantResults\011822 bna SIM1.batch.bin			✓	
CmdSaveBatchTable	BL2000\jheine	1/19/2022 8:56:55 AM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh011822\1 e8270c bna SIM\QuantResults\011822 bna SIM1.batch.bin			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:57:04 AM	Set SampleApproved = True for sample Jan1801.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:57:06 AM	Set SampleApproved = True for sample Jan1802.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:57:07 AM	Set SampleApproved = True for sample Jan1803.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:57:08 AM	Set SampleApproved = True for sample Jan1804.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:57:09 AM	Set SampleApproved = True for sample Jan1805.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:57:10 AM	Set SampleApproved = True for sample Jan1806.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:57:12 AM	Set SampleApproved = True for sample Jan1807.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:57:13 AM	Set SampleApproved = True for sample Jan1808.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:57:14 AM	Set SampleApproved = True for sample Jan1809.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:57:15 AM	Set SampleApproved = True for sample Jan1810.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:57:17 AM	Set SampleApproved = True for sample Jan1811.D; previous value = False			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:57:18 AM	Set SampleApproved = True for sample Jan1812.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:57:19 AM	Set SampleApproved = True for sample Jan1813.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:57:21 AM	Set SampleApproved = True for sample Jan1814.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:57:22 AM	Set SampleApproved = True for sample Jan1815.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:57:23 AM	Set SampleApproved = True for sample Jan1816.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:57:24 AM	Set SampleApproved = True for sample Jan1817.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:57:25 AM	Set SampleApproved = True for sample Jan1818.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:57:31 AM	Set SampleApproved = True for sample Jan1819.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:57:32 AM	Set SampleApproved = True for sample Jan1820.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:57:33 AM	Set SampleApproved = True for sample Jan1821.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:57:34 AM	Set SampleApproved = True for sample Jan1822.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:57:35 AM	Set SampleApproved = True for sample Jan1823.D; previous value = False			✓	
CmdSetSampleAttribute	BL2000\jheine	1/19/2022 8:57:37 AM	Set SampleApproved = True for sample Jan1824.D; previous value = False			✓	
CmdSaveBatchTable	BL2000\jheine	1/19/2022 8:57:39 AM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011822\1 e8270c bna SIM\QuantResults\011822 bna SIM1.batch.bin			✓	
CmdOpenBatchTable	BL2000\jheine	2/4/2022 4:47:02 PM	Open batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011822\1 e8270c bna SIM\011822 bna SIM1.batch.bin			✓	
CmdQuantitate	BL2000\jheine	2/4/2022 4:47:23 PM	Quantitate all compounds in all samples			✓	

Audit Trail report

Name	User	Time	Action	Reason	Comment	Succeed	Exception
CmdSaveBatchTable	BL2000\jheine	2/4/2022 4:47:26 PM	Save batch \\MASSHUNTER\Org\Data\SV5975.I\sh 011822\1 e8270c bna SIM\QuantResults\011822 bna SIM1.batch.bin			✓	
GenerateReport	BL2000\jheine	2/4/2022 4:57:13 PM	Generates report - Method: D:\Org\reports\GCMSSSEMI Report Templates\Tests_for_LevelIV\Env_Qua ntResults_wGraphics+Chromatogram. m, Output Path: \\MASSHUNTER\Org\Data\SV5975.I\sh 011822\1 e8270c bna SIM\QuantReports\			✓	



Analytical RunID SV5975.I_220114A Standards Traceability Report

Spike ID: sv100210

Spike Name: BNA 2nd source 200ug/mL

Prep Date: 3/22/2021

Exp Date: 1/15/2022

Department: GCMSSEMI

Vendor:

Lot Number:

Balance ID:

Comments:

Type: Secondary

Prep By: John P. Heine

Status:

Final Volume: 1 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Dichloromethane EA342	13510	540	uL	1/15/2022

Stock Source	Base Units	Amount Added
sv83409	ug/mL	0.1 mL
sv82908	ug/mL	0.02 mL
sv83008	ug/mL	0.1 mL
sv83408	ug/mL	0.2 mL
sv83407	ug/mL	0.04 mL



Analytical RunID SV5975.I_220114A Standards Traceability Report

Spike ID: sv100418

Spike Name: BNA mix 200 ug/mL

Prep Date: 6/2/2021

Exp Date: 3/31/2022

Department: GCMSSEMI

Vendor:

Lot Number:

Balance ID:

Comments:

Type: Secondary

Prep By: John P. Heine

Status: New

Final Volume: 1.5 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Dichloromethane EA342	13510	0.51	mL	3/31/2022

Stock Source	Base Units	Amount Added
sv82908	ug/mL	0.03 mL
sv83301	ug/mL	0.15 mL
sv83120	ug/mL	0.15 mL
sv83419	ug/mL	0.15 mL
sv82917	ug/mL	0.15 mL
sv83410	ug/mL	0.15 mL
sv83407	ug/mL	0.06 mL
sv83201	ug/mL	0.15 mL



Analytical RunID SV5975.I_220114A Standards Traceability Report

Spike ID: sv100506

Spike Name: BNA low 50 ug/mL

Prep Date: 6/2/2021

Exp Date: 3/31/2022

Department: GCMSSEMI

Vendor:

Lot Number:

Balance ID:

Comments:

Type: Secondary

Prep By: John P. Heine

Status: New

Final Volume: 0.8 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Dichloromethane EA342	13510	0.6	mL	3/31/2022

Stock Source	Base Units	Amount Added
sv100418	ug/mL	0.2 mL



Analytical RunID SV5975.I_220114A Standards Traceability Report

Spike ID: sv100703

Spike Name: BNA Internals 2000 ug/mL

Prep Date: 12/9/2021

Exp Date: 5/31/2022

Department: GCMSSEMI

Vendor: Chemservice

Lot Number: 8443500

Balance ID:

Comments:

Type: Secondary

Prep By: John P. Heine

Status: New

Final Volume: 2.12 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Dichloromethane EA342	13510	1.06	mL	5/31/2022

Stock Source	Base Units	Amount Added
sv83403	ug/mL	1.06 mL



Analytical RunID SV5975.I_220114A Standards Traceability Report

Spike ID: sv82908

Spike Name: AE surr

Prep Date: 4/10/2019

Exp Date: 3/31/2022

Department: GCMSSEMI

Vendor: Sigma-Aldrich

Lot Number: LRAC2239

Balance ID:

Comments:

Type: Primary

Prep By: Sean McGrew

Status: New

Final Volume: mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
EPA 8270 Acids Surrogate Spike Mix HC	11383		mL	3/31/2022
Stock Source	Base Units	Amount Added		



Analytical RunID SV5975.I_220114A Standards Traceability Report

Spike ID: sv83008

Spike Name: Benzidines

Prep Date: 8/6/2019

Exp Date: 12/21/2022

Department: GCMSSEMI

Vendor: AccuStandard

Lot Number: 218121353

Balance ID:

Comments: 11742

Type: Primary

Prep By: Sean McGrew

Status: New

Final Volume: 1 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
				12/21/2022
Stock Source	Base Units	Amount Added		



Analytical RunID SV5975.I_220114A Standards Traceability Report

Spike ID: sv83403

Spike Name: BNA Internals 4000ug/mL

Prep Date: 12/29/2020

Exp Date: 5/31/2022

Department: GCMSSEMI

Vendor: Chemservice

Lot Number: 10051700

Balance ID:

Comments:

Type: Primary

Prep By: John P. Heine

Status: New

Final Volume: 8 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Mixture #8-Internal Standards	13372	8	mL	5/31/2022
Stock Source	Base Units	Amount Added		



Analytical RunID SV5975.I_220114A Standards Traceability Report

Standard ID: sv83407

Standard Name: BN Surr 5000 ug/mL

Prep Date: 12/14/2020

Exp Date: 10/31/2026

Department: GCMSSEMI

Vendor: Restek

Lot Number: A0166081

Balance ID:

Comments:

Type: Primary

Prep By: John P. Heine

Status: New

Final Volume: 5 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
B/N Surrogate Mix (4/89 SOW)	13328	1	mL	10/31/2026
Stock Source	Base Units	Amount Added		



Analytical RunID SV5975.I_220114A Standards Traceability Report

Spike ID: sv83408

Spike Name: 625 LCS Spk

Prep Date: 2/9/2021

Exp Date: 2/2/2026

Department: GCMSPR

Vendor: Absolute Standards

Lot Number: 050120

Balance ID:

Comments: 12x1mL ampules

Type: Primary

Prep By: Ryan F. Bengel

Status: Open

Final Volume: 1 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
CLP Semi-Volatiel Calibration Standard	13539	1	mL	2/2/2026

Stock Source	Base Units	Amount Added
--------------	------------	--------------



Analytical RunID SV5975.I_220114A Standards Traceability Report

Standard ID: sv83409

Standard Name: Additional

Prep Date: 3/18/2021

Exp Date: 1/15/2022

Department: GCMSPR

Vendor: AccuStandard

Lot Number: 220021255

Balance ID:

Comments: 10x1 mL ampules 2000 ug/mL

Type: Primary

Prep By: Ryan F. Bengel

Status:

Final Volume: mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Custom Semi-Volatile Standard	13342	1	mL	1/15/2022

Stock Source	Base Units	Amount Added
--------------	------------	--------------

Handwritten signature

CERTIFICATE OF ANALYSIS

Catalog No: CLP-AS-10X
Description: Acid Surrogate
Lot: 220031065
Solvent: Methanol
Hazards: Refer to SDS for complete safety information

Date Certified: Mar 6, 2020
Expiration: Mar 6, 2023
Sample Size: 1 mL
Components: 3
Storage Condition: Ambient (>5 °C)



Signal Word: Danger


Certified Reference Material



Component	CAS #	Purity % (GC/MS)	Prepared Concentration ² (mg/mL)	Certified Analyte Concentration ¹ (mg/mL)
2-Fluorophenol	367-12-4	99.8	20.20	20.16
Phenol-d5	4165-62-2	99.9	20.05	20.03
2,4,6-Tribromophenol	118-79-6	99.9	20.19	20.17

ID #: 14527
Opened: _____
Acid Surrogate
Expires: 3/6/2023
Rec'd: 11/17/2021
Energy Laboratories Inc 1120 So. 27th Street
Billings MT 59107

A product with a suffix (-1A, -2B, etc. or -01, -02, etc.) on its lot number has had its expiration date extended and is identical to the same lot number without the suffix.
² All weights are traceable through NIST, Test No. 684/289871-17
¹ Certified Analyte Concentration = Purity x Prepared Concentration.
The Uncertainty associated with the certified concentration reported on this certificate is ±2.4%. This value is the combined expanded uncertainty and represents an estimated standard deviation equal to the positive square root of the total variation of the uncertainty of components. A normal distribution is assumed and a coverage factor of K=2 is chosen using approximately a 95% confidence level.
Labels and certificates follow U.S. Conventions in reporting numerical values: A comma (,) is used to separate units of one-thousand or greater. A period (.) is used as a decimal place marker.
The information on this certificate may not be reproduced without the express permission of the manufacturer. See reverse side for additional information
Hazard Information: Please refer to the SDS for information regarding the hazards associated with using this material.
This product was prepared according to in-house procedures and is guaranteed to be homogeneous.

Certified By: 
Larry Decker, Organic QC Manager

For use in routine laboratory analysis.



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31086 **Lot No.:** A0175748

Description : B/N Surrogate Mix (4/89 SOW)
Base Neutral Surrogate 5000µg/mL, Methylene Chloride, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : July 31, 2027 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

ID #: 14431

Opened: _____
B/N Surrogate Mix (4/89 SOW)
Expires: 7/31/2027
Rec'd: 10/25/2021
Energy Laboratories Inc. 1120 So. 27th Street
Billings MT 59107

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)	
1	Nitrobenzene-d5 CAS # 4165-60-0 Purity 99% (Lot PR-29940A)	5,027.3 µg/mL	+/- 29.2293 µg/mL	Gravimetric
			+/- 226.4341 µg/mL	Unstressed
			+/- 251.2566 µg/mL	Stressed
2	2-Fluorobiphenyl CAS # 321-60-8 Purity 99% (Lot 00019169)	5,001.1 µg/mL	+/- 29.0767 µg/mL	Gravimetric
			+/- 225.2518 µg/mL	Unstressed
			+/- 249.9447 µg/mL	Stressed
3	p-Terphenyl-d14 CAS # 1718-51-0 Purity 99% (Lot PR-30504)	5,001.4 µg/mL	+/- 29.0787 µg/mL	Gravimetric
			+/- 225.2668 µg/mL	Unstressed
			+/- 249.9613 µg/mL	Stressed

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

Tech Tips:

Due to the limited solubility of p-terphenyl-d14 in methanol, we do not recommend that this mixture be diluted in methanol.

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

330°C

Det. Type:

FID



This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Sam Moodler
Sam Moodler - Operations Tech I

Date Mixed: 25-Aug-2021

Balance: B345965662

Marline Cowan
Marline Cowan - Operations Tech I

Date Passed: 27-Aug-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value (includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at www.restek.com/Contact-Us for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at www.restek.com/Contact-Us.
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.



CERTIFIED WEIGHT REPORT

Part Number: **92180**
Lot Number: **091521**
Description: **CLP Semi-Volatile Calibration Standard**
64 components
Expiration Date: **091526**
Recommended Storage: **Freezer (0 °C)**
Nominal Concentration (µg/mL): **1000**
NIST Test ID#: **6UTB**

Solvent: **Methylene chloride**
Lot#: **104929**


Formulated By: <i>Prashant Chauhan</i>	091521 DATE
Reviewed By: <i>Pedro L. Rentas</i>	091521 DATE

Weight(s) shown below were combined and diluted to (mL):
100.0 0.003 5E-05 Balance Uncertainty
Flask Uncertainty

Compound	(RM#)	Lot Number	Dil. Factor	Initial Vol. (mL)	Initial Conc. (µg/mL)	Nominal Conc. (µg/mL)	Purity (%)	Uncertainty Purity (%)	Uncertainty Pipette (mL)	Target Weight(g)	Actual Weight(g)	Actual Conc. (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information (Solvent Safety Info. On Attached pg.)		
														CAS#	OSHA PEL (TWA)	LOSO
1. 2,2'-Oxybis(1-chloropropane)	(0078)	012016AR	NA	NA	NA	1000	98.9	0.2	NA	0.10112	0.10129	1001.7	4.2	108-60-1	N/A	ori-rat 240mg/kg
2. Hexachlorobenzene	(0195)	051697	NA	NA	NA	1000	99	0.2	NA	0.10102	0.10128	1002.6	4.2	118-74-1	N/A	ori-rat 10µg/kg
3. bis(2-Chloroethoxy) methane	10111	011214	0.05	5.00	20018.4	1000	NA	NA	0.017	NA	NA	1000.8	8.0	111-91-1	N/A	ori-rat 10µg/kg
4. bis(2-Chloroethyl) ether	10111	011214	0.05	5.00	20014.3	1000	NA	NA	0.017	NA	NA	1000.5	8.0	111-44-4	15 ppm (90mg/m3/8H)(skin)	ori-rat 75mg/kg
5. bis(2-Ethylhexyl) phthalate	10111	011214	0.05	5.00	20008.8	1000	NA	NA	0.017	NA	NA	1000.3	8.0	117-81-7	5mg/m3/8H	ori-rat 30600mg/kg
6. 4-Bromophenyl phenyl ether	10111	011214	0.05	5.00	20011.3	1000	NA	NA	0.017	NA	NA	1000.5	8.0	101-55-3	N/A	ori-rat 2330mg/kg
7. Benzyl butyl phthalate	10111	011214	0.05	5.00	20009.5	1000	NA	NA	0.017	NA	NA	1000.4	8.0	7005-72-3	N/A	ori-rat 2330mg/kg
8. 4-Chlorophenyl phenyl ether	10111	011214	0.05	5.00	20015.7	1000	NA	NA	0.017	NA	NA	1000.7	8.0	84-66-2	5mg/m3/8H	ori-rat 8600mg/kg
9. Diethyl phthalate	10111	011214	0.05	5.00	20011.6	1000	NA	NA	0.017	NA	NA	1000.5	8.0	131-11-3	5mg/m3/8H	ori-rat 6800mg/kg
10. Dimethyl phthalate	10111	011214	0.05	5.00	20012.2	1000	NA	NA	0.017	NA	NA	1000.5	8.0	84-74-2	5mg/m3/8H	ori-rat 8000mg/kg
11. Di-n-butyl phthalate	10111	011214	0.05	5.00	20010.0	1000	NA	NA	0.017	NA	NA	1000.4	8.0	117-84-0	N/A	ori-rat 47000mg/kg
12. Di-n-octyl phthalate	10111	011214	0.05	5.00	20010.5	1000	NA	NA	0.017	NA	NA	1000.4	8.0	62-75-9	N/A	ori-rat 58mg/kg
13. N-Nitrosodimethylamine	10112	042820	0.05	5.00	20003.9	1000	NA	NA	0.017	NA	NA	1000.1	8.1	103-33-3	N/A	ori-rat 1000mg/kg
14. N-Nitroso-n-propylamine	10112	042820	0.05	5.00	20005.4	1000	NA	NA	0.017	NA	NA	1000.0	8.0	91-58-7	N/A	ori-rat 2078mg/kg
15. 1,2-Diphenylhydrazine (as Azobenzene)	10112	042820	0.05	5.00	20003.7	1000	NA	NA	0.017	NA	NA	1000.2	8.0	95-50-1	50 ppm (300mg/m3) (CL)	ori-rat 500mg/kg
16. 2-Chloronaphthalene	10112	042820	0.05	5.00	20005.4	1000	NA	NA	0.017	NA	NA	1000.1	8.0	541-73-1	N/A	ipr-mus 1062mg/kg
17. 1,2-Dichlorobenzene	10112	042820	0.05	5.00	20003.3	1000	NA	NA	0.017	NA	NA	1000.2	8.0	106-46-7	75 ppm (450mg/m3/8H)	ori-rat 500mg/kg
18. 1,3-Dichlorobenzene	10112	042820	0.05	5.00	20002.4	1000	NA	NA	0.017	NA	NA	1000.1	8.1	121-14-2	1.5mg/m3/8H (skin)	ori-rat 268mg/kg
19. 1,4-Dichlorobenzene	10112	042820	0.05	5.00	20001.8	1000	NA	NA	0.017	NA	NA	1000.4	12.4	87-68-3	0.02 ppm (0.24mg/m3/8H)	ori-rat 82mg/kg
20. 2,4-Dinitrotoluene	10112	042820	0.05	5.00	20002.4	1000	NA	NA	0.017	NA	NA	1000.0	8.0	77-47-4	0.01 ppm (0.1mg/m3/8H)	ori-rat 1300mg/kg
21. 2,6-Dinitrotoluene	10112	042820	0.05	5.00	20009.4	1000	NA	NA	0.017	NA	NA	1000.0	8.0	87-68-3	0.02 ppm (0.24mg/m3/8H)	ori-rat 82mg/kg
22. Hexachloro-1,3-butadiene	10112	042820	0.05	5.00	20001.8	1000	NA	NA	0.017	NA	NA	1000.0	8.0	67-72-1	1 ppm (10mg/m3/8H)(skin)	ori-rat 4970mg/kg
23. Hexachlorocyclopentadiene	10112	042820	0.05	5.00	20002.4	1000	NA	NA	0.017	NA	NA	1000.1	8.1	78-59-1	25 ppm	ori-rat 2330mg/kg
24. Hexachloroethane	10112	042820	0.05	5.00	20002.0	1000	NA	NA	0.017	NA	NA	1000.1	8.0	98-95-3	1 ppm (5mg/m3/8H)(skin)	ori-rat 780mg/kg
25. Isophorone	10112	042820	0.05	5.00	20010.2	1000	NA	NA	0.017	NA	NA	1000.0	8.0	120-82-1	5 ppm (CL) (40mg/3)	ori-rat 756mg/kg
26. Nitrobenzene	10112	042820	0.05	5.00	20061.2	1000	NA	NA	0.017	NA	NA	1000.4	8.0	95-48-7	5 ppm (22mg/m3/8H)(skin)	ori-rat 121mg/kg
27. 1,2,4-Trichlorobenzene	10114	081919	0.05	5.00	20023.2	1000	NA	NA	0.017	NA	NA	1003.0	8.0	106-44-5	5 ppm (22mg/m3/8H)(skin)	ori-rat 207mg/kg
28. o-Cresol (2-Methylphenol)	10115	060512	0.05	5.00	20009.6	1000	NA	NA	0.017	NA	NA	1001.1	8.0	95-95-4	N/A	ori-rat 820mg/kg
29. p-Cresol (4-Methylphenol)	10115	060512	0.05	5.00	20020.2	1000	NA	NA	0.017	NA	NA	1000.9	8.0	106-47-8	N/A	ori-rat 310mg/kg
30. 2,4,5-Trichlorophenol	10115	060512	0.05	5.00	20012.9	1000	NA	NA	0.017	NA	NA	1000.5	8.1	132-64-9	N/A	ori-rat 1630mg/kg
31. 4-Chloroaniline	10115	060512	0.05	5.00	20011.8	1000	NA	NA	0.017	NA	NA	1000.5	8.0	91-57-6	N/A	ori-rat 1600mg/kg
32. Dibenzofuran	10115	060512	0.05	5.00	20018.6	1000	NA	NA	0.017	NA	NA	1000.8	8.0	88-74-4	N/A	ori-rat 535mg/kg
33. 2-Methylnaphthalene	10115	060512	0.05	5.00	20014.9	1000	NA	NA	0.017	NA	NA	1000.8	8.0	99-09-2	N/A	ori-rat 750mg/kg
34. 2-Nitroaniline	10118	072120	0.05	5.00	20003.9	1000	NA	NA	0.017	NA	NA	1000.8	8.0	100-01-6	1 ppm (6mg/m3/8H)(skin)	ori-rat 1830mg/kg
35. 3-Nitroaniline	10118	072120	0.05	5.00	20002.9	1000	NA	NA	0.017	NA	NA	1000.1	8.0	59-50-7	N/A	ori-rat 670mg/kg
36. 4-Nitroaniline	10118	072120	0.05	5.00	20003.1	1000	NA	NA	0.017	NA	NA	1000.0	8.0	95-57-8	N/A	ori-rat 580mg/kg
37. 4-Chloro-3-methylphenol	10118	072120	0.05	5.00	20003.3	1000	NA	NA	0.017	NA	NA	1000.1	8.1	105-67-9	N/A	ori-rat 3200mg/kg
38. 2-Chlorophenol	10118	072120	0.05	5.00	20001.8	1000	NA	NA	0.017	NA	NA	1000.0	8.0	51-28-5	N/A	ori-rat 30mg/kg
39. 2,4-Dichlorophenol	10118	072120	0.05	5.00	20002.5	1000	NA	NA	0.017	NA	NA	1000.0	8.0	88-75-5	N/A	ori-rat 334mg/kg
40. 2,4-Dimethylphenol	10118	072120	0.05	5.00	20002.0	1000	NA	NA	0.017	NA	NA	1000.0	8.0	100-02-7	N/A	ori-rat 250mg/kg
41. 2,4-Dinitrophenol	10118	072120	0.05	5.00	20003.9	1000	NA	NA	0.017	NA	NA	1000.0	8.0	87-86-5	0.5mg/m3/8H (skin)	ori-rat 27mg/kg
42. 4,6-Dinitro-2-methylphenol	10118	072120	0.05	5.00	20004.2	1000	NA	NA	0.017	NA	NA	1000.1	8.0	108-95-2	5 ppm (19mg/m3/8H)(skin)	ori-rat 317mg/kg
43. 2-Nitrophenol	10118	072120	0.05	5.00	20001.2	1000	NA	NA	0.018	NA	NA	1000.5	4.1	83-32-9	N/A	ori-rat 820mg/kg
44. 4-Nitrophenol	10118	072120	0.05	5.00	20002.0	1000	NA	NA	0.018	NA	NA	1000.0	4.2	208-96-8	N/A	ori-rat 800mg/kg
45. Pentachlorophenol	10118	072120	0.05	5.00	20003.7	1000	NA	NA	0.018	NA	NA	1000.0	4.1	120-12-7	0.2mg/m3 (8H)	ipr-mus 430mg/kg
46. Phenol	10118	072120	0.05	5.00	20001.3	1000	NA	NA	0.018	NA	NA	1000.6	4.2	56-55-3	N/A	ori-rat 200mg/kg
47. 2,4,6-Trichlorophenol	10118	072120	0.05	5.00	2000.9	1000	NA	NA	0.018	NA	NA	999.9	4.1	50-32-8	0.2mg/m3 (8H)	scu-rat 50mg/kg
48. Acenaphthene	1007	042420	0.50	50.00	2000.0	1000	NA	NA	0.018	NA	NA	1000.4	4.1	205-99-2	N/A	ori-rat 200mg/kg
49. Acenaphthylene	1007	042420	0.50	50.00	2000.9	1000	NA	NA	0.018	NA	NA	1000.5	4.1	207-08-9	N/A	ori-rat 200mg/kg
50. Anthracene	1007	042420	0.50	50.00	2001.2	1000	NA	NA	0.018	NA	NA	1000.5	4.1	191-24-2	N/A	ori-rat 200mg/kg
51. Benzo(a)anthracene	1007	042420	0.50	50.00	2000.3	1000	NA	NA	0.018	NA	NA	1000.4	4.1	86-74-8	N/A	ipr-mus 200mg/kg
52. Benzo(a)pyrene	1007	042420	0.50	50.00	2000.8	1000	NA	NA	0.018	NA	NA	1000.3	4.2	218-01-9	0.2mg/m3	ori-rat 200mg/kg
53. Benzo(b)fluoranthene	1007	042420	0.50	50.00	2000.3	1000	NA	NA	0.018	NA	NA	1000.3	4.2	53-70-3	0.2mg/m3	ori-rat 200mg/kg
54. Benzo(k)fluoranthene	1007	042420	0.50	50.00	2000.9	1000	NA	NA	0.018	NA	NA	1000.4	4.2	206-44-0	N/A	ori-rat 2000mg/kg
55. Benzo(g,h)perylene	1007	042420	0.50	50.00	2000.1	1000	NA	NA	0.018	NA	NA	1000.3	4.2	86-73-7	N/A	ori-rat 2000mg/kg
56. Carbazole	1007	042420	0.50	50.00	2000.9	1000	NA	NA	0.018	NA	NA	1000.4	4.1	193-39-5	N/A	ori-rat 490mg/kg
57. Chrysene	1007	042420	0.50	50.00	2000.9	1000	NA	NA	0.018	NA	NA	1000.4	4.1	91-20-3	10 ppm (50mg/m3/8H)	ori-rat 490mg/kg
58. Dibenzo(a,h)anthracene	1007	042420	0.50	50.00	2000.9	1000	NA	NA	0.018	NA	NA	1000.4	4.1	85-01-8	0.2mg/m3/8H	ori-rat 700mg/kg
59. Fluoranthene	1007	042420	0.50	50.00	2001.0	1000	NA	NA	0.018	NA	NA	1000.4	4.2	129-00-0	0.2mg/m3/8H	ori-rat 2700mg/kg
60. Fluorene	1007	042420	0.50	50.00	2001.0	1000	NA	NA	0.018	NA	NA	1000.4	4.2	129-00-0</		



Method GC8MSD-2.M: Column:SBB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (14 min.), Rate = 10°C/min., Injector B = 250°C, Detector B = 290°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by Melissa Stonier.

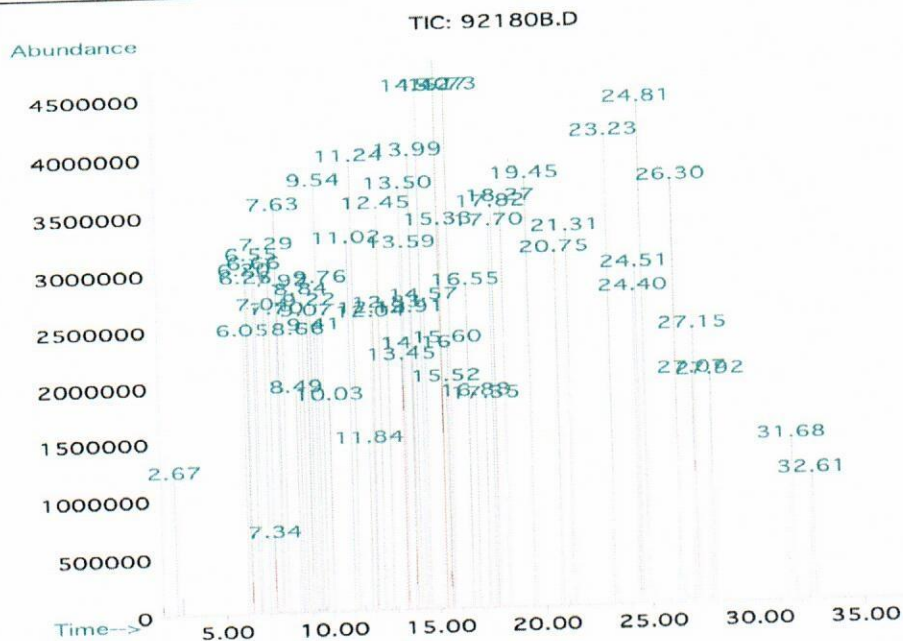

Peak No	Name	MSD RT (min.)
1	N-nitrosodimethylamine	2.67
2	Phenol	6.05
3	bis(2-Chloroethyl)ether	6.20
4	2-Chlorophenol	6.26
5	1,3-Dichlorobenzene	6.55
6	1,4-Dichlorobenzene	6.63
7	1,2-Dichlorobenzene	7.04
8	o-Cresol (2-methylphenol)	7.29
9	bis(2-Chloroisopropyl)ether	7.34
10	p-Cresol (4-methylphenol)/N-nitrosodi-n-propylamine	7.63
11	Hexachloroethane	7.70
12	Nitrobenzene	7.92
13	Isophorone	8.49
14	2-Nitrophenol	8.66
15	2,4-Dimethylphenol	8.84
16	bis(2-Chloroethoxy)methane	9.07
17	2,4-Dichlorophenol	9.22
18	1,2,4-Trichlorobenzene	9.41
19	Naphthalene	9.54
20	4-Chloroaniline	9.76
21	Hexachloro-1,3-Butadiene	10.03
22	4-Chloro-3-methylphenol	11.02
23	2-Methylnaphthalene	11.24
24	Hexachlorocyclopentadiene	11.84
25	2,4,6-Trichlorophenol	12.13
26	2,4,5-Trichlorophenol	12.45
27	2-Chloronaphthalene	12.84
28	2-Nitroaniline	13.45
29	Dimethyl phthalate	13.50
30	Acenaphthylene	13.59
31	2,6-Dinitrotoluene	13.91
32	3-Nitroaniline	13.99
33	Acenaphthene	14.16
34	2,4-Dinitrophenol	14.40
35	Dibenzofuran/4-Nitrophenol	14.57
36	2,4-Dinitrotoluene	15.27
37	Diethyl phthalate/fluorene	15.33
38	4-Chlorophenyl phenyl ether	15.52
39	4-Nitroaniline	15.60
40	4,6-Dinitro-2-methylphenol	15.73
41	Azobenzene	16.56
42	4-Bromophenyl phenyl ether	16.89
43	Hexachlorobenzene	17.70
44	Pentachlorophenol	17.82
45	Phenanthrene	18.27
46	Anthracene	19.45
47	Carbazole	20.75
48	Di-n-butyl phthalate	21.31
49	Fluoranthene	23.23
50	Pyrene	24.40
51	Benzyl butyl phthalate	24.51
52	Benzo(a)anthracene	24.82
53	Chrysene	26.30
54	bis(2-Ethylhexyl)phthalate	27.07
55	Di-n-octyl phthalate	27.15
56	Benzo(b)fluoranthene	27.92
57	Benzo(k)fluoranthene	31.68
58	Benzo(a)pyrene	32.61
59	Indeno(1,2,3-cd)pyrene/Dibenz(a,h)anthracene	
60	Benzo(g,h,i)perylene	

CERTIFICATE OF ANALYSIS

Catalog No: S-14500-R2
Description: Custom Semi-Volatile Standard
Lot: 220021255-02
Solvent: Dichloromethane
Hazards: Refer to SDS for complete safety information

Date Certified: Aug 31, 2021
Expiration: Oct 1, 2022
Sample Size: 1 mL
Components: 10
Storage Condition: Freeze (<-10 °C)/Sonicate



Signal Word: Warning

Certified Reference Material



AR-1463

Component	CAS #	Purity % (GC/MS)	Prepared Concentration ² (µg/mL)	Certified Analyte Concentration ¹ (µg/mL)
Pyridine				
4-Chlorophenol	110-86-1	98.7	2026	2000
1-Methylnaphthalene	106-48-9	100.0	2019	2019
N-Nitrosodiphenylamine	90-12-0	98.5	2003	1973
4-Chloro-2-methylphenol	86-30-6	100.0	2022	2022
Benzoic acid	1570-64-5	97.0	2069*	2007
Aniline	65-85-0	99.5	2010	2000
Benzyl alcohol	62-53-3	98.0	2002	1962
Triallate	100-51-6	99.9	2011	2009
o-Terphenyl	2303-17-5	99.9	2013	2011
	84-15-1	99.9	2019	2017

ID #: 14279
Opened: _____
Custom Semi-Volatile Standard
Expires: 10/1/2022
Rec'd: 9/16/2021
Enerav Laboratories Inc 1120 So. 27th Street
Billings MT 59107

This Certified Reference Material was verified in accordance with ISO/IEC 17025

* Weight compensated to 100% purity.

A product with a suffix (-1A, -2B, etc. or -01, -02, etc.) on its lot number has had its expiration date extended and is identical to the same lot number without the suffix.

² All weights are traceable through NIST, Test No. 684/289871-17

¹ Certified Analyte Concentration = Purity x Prepared Concentration.


The Uncertainty associated with the certified concentration reported on this certificate is ±2.4%. This value is the combined expanded uncertainty and represents an estimated standard deviation equal to the positive square root of the total variation of the uncertainty of components. A normal distribution is assumed and a coverage factor of K=2 is chosen using approximately a 95% confidence level.

Labels and certificates follow U.S. Conventions in reporting numerical values: A comma (,) is used to separate units of one-thousand or greater. A period (.) is used as a decimal place marker.

The information on this certificate may not be reproduced without the express permission of the manufacturer. See reverse side for additional information

Hazard Information: Please refer to the SDS for information regarding the hazards associated with using this material.

This product was prepared according to in-house procedures and is guaranteed to be homogeneous.

Certified By: 
Larry Decker, Organic QC Manager

CERTIFICATE OF ANALYSIS

Catalog No: S-6237B
Description: Custom Semivolatile STD
Lot: 221111080
Solvent: Dichloromethane
Hazards: Refer to SDS for complete safety information

Date Certified: Nov 5, 2021
Expiration: Dec 5, 2022
Sample Size: 1 mL
Components: 29
Storage Condition: Freeze (<-10 °C)



Certified Reference Material



Component	CAS #	Purity % (GC/MS)	Prepared Concentration ² (µg/mL)	Certified Analyte Concentration ¹ (µg/mL)
2-Acetamidofluorene	53-96-3	100.0	2026	2026
Aramite	140-57-8	100.0	2013	2013
Chlorobenzilate	510-15-6	100.0	2001	2001
Diallate	2303-16-4	97.5	2062*	2010
Dibenzofuran	132-64-9	100.0	2007	2007
2,6-Dichlorophenol	87-65-0	100.0	2005	2005
Dimethoate	60-51-5	99.1	2011	1993
7,12-Dimethylbenz(a)anthracene	57-97-6	100.0	2011	2011
1,3-Dinitrobenzene	99-65-0	99.9	2009	2007
Disulfoton	298-04-4	100.0	2027	2027
Ethyl methanesulfonate	62-50-0	100.0	2011	2011
Famphur	52-85-7	99.3	2011	1997
Hexachlorophene	70-30-4	98.0	2034	1993
Hexachloropropene	1888-71-7	97.9	2046*	2003
Isosafrole **	120-58-1	98.1	2025	1987
Methapyrilene	91-80-5	98.8	2013	1989
3-Methylcholanthrene	56-49-5	99.0	2033	2013
Methyl methanesulfonate	66-27-3	100.0	2006	2006
Methyl parathion	298-00-0	99.9	2016	2014
1,4-Naphthoquinone	130-15-4	100.0	2022	2022
Parathion	56-38-2	99.6	2008	2000
Pentachlorobenzene	608-93-5	99.0	2017	1997
Phorate	298-02-2	97.8	2072*	2026
Safrole	94-59-7	98.2	2033	1996
Sulfotep	3689-24-5	98.8	2026	2002
1,2,4,5-Tetrachlorobenzene	95-94-3	100.0	2001	2001
2,3,4,6-Tetrachlorophenol	58-90-2	95.3	2113*	2014
Thionazin	297-97-2	97.0	2066*	2004
O,O,O-Triethylphosphorothioate	126-68-1	100.0	2007	2007

ID #: 14503
Opened: _____
Custom SemiVolatile Standard
Expires: 12/5/2022
Rec'd: 11/9/2021
Enerav Laboratories Inc 1120 So. 27th Street
Billings MT 59107

CERTIFICATE OF ANALYSIS

Catalog No: S-6237B
Description: Custom Semivolatile STD
Lot: 221111080
Solvent: Dichloromethane

Date Certified: Nov 5, 2021
Expiration: Dec 5, 2022
Sample Size: 1 mL
Components: 29

This Certified Reference Material was verified in accordance with ISO/IEC 17025

* Weight compensated to 100% purity.

**Mixture of isomers (75.7% Cis + 22.4 % Trans)

A product with a suffix (-1A, -2B, etc. or -01, -02, etc.) on its lot number has had its expiration date extended and is identical to the same lot number without the suffix.

² All weights are traceable through NIST, Test No. 684/289871-17

¹ Certified Analyte Concentration = Purity x Prepared Concentration.


The Uncertainty associated with the certified concentration reported on this certificate is $\pm 2.4\%$. This value is the combined expanded uncertainty and represents an estimated standard deviation equal to the positive square root of the total variation of the uncertainty of components. A normal distribution is assumed and a coverage factor of K=2 is chosen using approximately a 95% confidence level.

Labels and certificates follow U.S. Conventions in reporting numerical values: A comma (,) is used to separate units of one-thousand or greater. A period (.) is used as a decimal place marker.

The information on this certificate may not be reproduced without the express permission of the manufacturer. See reverse side for additional information

Hazard Information: Please refer to the SDS for information regarding the hazards associated with using this material.

This product was prepared according to in-house procedures and is guaranteed to be homogeneous.

Certified By: 

Larry Decker, Organic QC Manager

ID #: 13755

Opened: _____

Acetone DZ963

Expires: 9/24/2022

Rec'd: 4/13/2021

Energy Laboratories Inc 1120 So. 27th Street
Billings MT 59107

Honeywell

CERTIFICATE OF ANALYSIS

Honeywell Burdick & Jackson®

1953 South Harvey Street
Muskegon, MI 49442
Phone: (800) 368-0050
Fax: (231) 728-8226
lab.honeywell.com

Brand: Research Chemicals - B&J
Product: 010
Lot No.: DZ963
Production Date: 24-Sep-2020
Best Before: 24-Sep-2022

Acetone, B&J Brand™, >99.9%
for HPLC, GC, pesticide residue analysis and spectrophotometry

Parameter	Specification		Result	Units
	Min.	Max.		
Water by Karl Fischer Titration		0.50	0.45	%
UV Cutoff		330	328	nm
Refractive Index (20°C)	1.3583	1.3589	1.3585	
Residue		1	<0.5	mg/L
GC Analysis (excluding water)	99.9		99.98	%
Electron Capture GC		10	<10	ng/L
UV Absorbance @ 340 nm		0.060	0.0482	AU
UV Absorbance @ 350 nm		0.010	0.0047	AU
UV Absorbance @ 375 nm		0.005	<0.0001	AU
UV Absorbance @ 400 nm		0.005	<0.0001	AU

Honeywell
Quality Control Approval

Muskegon 9/24/2020 LIMS Sample No.: AL03008



Analytical RunID SV5975.I_220114A Standards Traceability Report

Spike ID: sv100210

Spike Name: BNA 2nd source 200ug/mL

Prep Date: 3/22/2021

Exp Date: 1/15/2022

Department: GCMSSEMI

Vendor:

Lot Number:

Balance ID:

Comments:

Type: Secondary

Prep By: John P. Heine

Status:

Final Volume: 1 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Dichloromethane EA342	13510	540	uL	1/15/2022

Stock Source	Base Units	Amount Added
sv83409	ug/mL	0.1 mL
sv82908	ug/mL	0.02 mL
sv83008	ug/mL	0.1 mL
sv83408	ug/mL	0.2 mL
sv83407	ug/mL	0.04 mL



Analytical RunID SV5975.I_220114A Standards Traceability Report

Spike ID: sv100418

Spike Name: BNA mix 200 ug/mL

Prep Date: 6/2/2021

Exp Date: 3/31/2022

Department: GCMSSEMI

Vendor:

Lot Number:

Balance ID:

Comments:

Type: Secondary

Prep By: John P. Heine

Status: New

Final Volume: 1.5 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Dichloromethane EA342	13510	0.51	mL	3/31/2022

Stock Source	Base Units	Amount Added
sv82908	ug/mL	0.03 mL
sv83301	ug/mL	0.15 mL
sv83120	ug/mL	0.15 mL
sv83419	ug/mL	0.15 mL
sv82917	ug/mL	0.15 mL
sv83410	ug/mL	0.15 mL
sv83407	ug/mL	0.06 mL
sv83201	ug/mL	0.15 mL



Analytical RunID SV5975.I_220114A Standards Traceability Report

Spike ID: sv100506

Spike Name: BNA low 50 ug/mL

Prep Date: 6/2/2021

Exp Date: 3/31/2022

Department: GCMSSEMI

Vendor:

Lot Number:

Balance ID:

Comments:

Type: Secondary

Prep By: John P. Heine

Status: New

Final Volume: 0.8 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Dichloromethane EA342	13510	0.6	mL	3/31/2022

Stock Source	Base Units	Amount Added
sv100418	ug/mL	0.2 mL



Analytical RunID SV5975.I_220114A Standards Traceability Report

Spike ID: sv100703

Spike Name: BNA Internals 2000 ug/mL

Prep Date: 12/9/2021

Exp Date: 5/31/2022

Department: GCMSSEMI

Vendor: Chemservice

Lot Number: 8443500

Balance ID:

Comments:

Type: Secondary

Prep By: John P. Heine

Status: New

Final Volume: 2.12 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Dichloromethane EA342	13510	1.06	mL	5/31/2022

Stock Source	Base Units	Amount Added
sv83403	ug/mL	1.06 mL



Analytical RunID SV5975.I_220114A Standards Traceability Report

Spike ID: sv82908

Spike Name: AE surr

Prep Date: 4/10/2019

Exp Date: 3/31/2022

Department: GCMSSEMI

Vendor: Sigma-Aldrich

Lot Number: LRAC2239

Balance ID:

Comments:

Type: Primary

Prep By: Sean McGrew

Status: New

Final Volume: mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
EPA 8270 Acids Surrogate Spike Mix HC	11383		mL	3/31/2022
Stock Source	Base Units	Amount Added		



Analytical RunID SV5975.I_220114A Standards Traceability Report

Spike ID: sv83008

Spike Name: Benzidines

Prep Date: 8/6/2019

Exp Date: 12/21/2022

Department: GCMSSEMI

Vendor: AccuStandard

Lot Number: 218121353

Balance ID:

Comments: 11742

Type: Primary

Prep By: Sean McGrew

Status: New

Final Volume: 1 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
				12/21/2022
Stock Source	Base Units	Amount Added		



Analytical RunID SV5975.I_220114A Standards Traceability Report

Spike ID: sv83403

Spike Name: BNA Internals 4000ug/mL

Prep Date: 12/29/2020

Exp Date: 5/31/2022

Department: GCMSSEMI

Vendor: Chemservice

Lot Number: 10051700

Balance ID:

Comments:

Type: Primary

Prep By: John P. Heine

Status: New

Final Volume: 8 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Mixture #8-Internal Standards	13372	8	mL	5/31/2022
Stock Source	Base Units	Amount Added		



Analytical RunID SV5975.I_220114A Standards Traceability Report

Standard ID: sv83407

Standard Name: BN Surr 5000 ug/mL

Prep Date: 12/14/2020

Exp Date: 10/31/2026

Department: GCMSSEMI

Vendor: Restek

Lot Number: A0166081

Balance ID:

Comments:

Type: Primary

Prep By: John P. Heine

Status: New

Final Volume: 5 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
B/N Surrogate Mix (4/89 SOW)	13328	1	mL	10/31/2026
Stock Source	Base Units	Amount Added		



Analytical RunID SV5975.I_220114A Standards Traceability Report

Spike ID: sv83408

Spike Name: 625 LCS Spk

Prep Date: 2/9/2021

Exp Date: 2/2/2026

Department: GCMSPR

Vendor: Absolute Standards

Lot Number: 050120

Balance ID:

Comments: 12x1mL ampules

Type: Primary

Prep By: Ryan F. Benge

Status: Open

Final Volume: 1 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
CLP Semi-Volatiel Calibration Standard	13539	1	mL	2/2/2026

Stock Source	Base Units	Amount Added
--------------	------------	--------------



Analytical RunID SV5975.I_220114A Standards Traceability Report

Standard ID: sv83409

Standard Name: Additional

Prep Date: 3/18/2021

Exp Date: 1/15/2022

Department: GCMSPR

Vendor: AccuStandard

Lot Number: 220021255

Balance ID:

Comments: 10x1 mL ampules 2000 ug/mL

Type: Primary

Prep By: Ryan F. Bengel

Status:

Final Volume: mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Custom Semi-Volatile Standard	13342	1	mL	1/15/2022

Stock Source	Base Units	Amount Added
--------------	------------	--------------

CERTIFICATE OF ANALYSIS

Catalog No: S-14500-R2
Description: Custom Semi-Volatile Standard
Lot: 220021255-01
Solvent: Dichloromethane
Hazards: Refer to SDS for complete safety information

Date Certified: Dec 15, 2020
Expiration: Jan 15, 2022
Sample Size: 1 mL
Components: 10
Storage Condition: Freeze (<-10 °C)/Sonicate



Certified Reference Material



Component	CAS #	Purity % (GC/MS)	Prepared Concentration ² (µg/mL)	Certified Analyte Concentration ¹ (µg/mL)
Pyridine	110-86-1	98.7	2026	2000
4-Chlorophenol	106-48-9	100.0	2019	2019
1-Methylnaphthalene	90-12-0	98.5	2003	1973
N-Nitrosodiphenylamine	86-30-6	100.0	2022	2022
4-Chloro-2-methylphenol	1570-64-5	97.0	2069*	2007
Benzoic acid	65-85-0	99.5	2010	2000
Aniline	62-53-3	98.0	2002	1962
Benzyl alcohol	100-51-6	99.9	2011	2009
Triallate	2303-17-5	99.9	2013	2011
o-Terphenyl	84-15-1	99.9	2019	2017

ID #: 13342

Opened:

Custom Semi-Volatile Standard

Expires: 1/15/2022

Rec'd: 12/17/2020

Energry Laboratories Inc 1120 So. 27th Street
Billings MT 59107

* Weight compensated to 100% purity.

A product with a suffix (-1A, -2B, etc. or -01, -02, etc.) on its lot number has had its expiration date extended and is identical to the same lot number without the suffix.

² All weights are traceable through NIST, Test No. 684/289871-17

¹ Certified Analyte Concentration = Purity x Prepared Concentration.

The Uncertainty associated with the certified concentration reported on this certificate is $\pm 2.4\%$. This value is the combined expanded uncertainty and represents an estimated standard deviation equal to the positive square root of the total variation of the uncertainty of components. A normal distribution is assumed and a coverage factor of K=2 is chosen using approximately a 95% confidence level.

Labels and certificates follow U.S. Conventions in reporting numerical values: A comma (,) is used to separate units of one-thousand or greater. A period (.) is used as a decimal place marker.

The information on this certificate may not be reproduced without the express permission of the manufacturer. See reverse side for additional information

Hazard Information: Please refer to the SDS for information regarding the hazards associated with using this material.

This product was prepared according to in-house procedures and is guaranteed to be homogeneous.

Certified By:



Larry Decker, Organic QC Manager

For use in routine laboratory analysis.

Certificate of Analysis

EPA 8270 ACIDS SURROGATE SPIKE MIX
HC,1X1ML,10MG/ML,METHANOL


*Certified
Reference
Material*

Description

Product ID 47260-U
Lot LRAC2239
Expiration Date March 2022
Manufacturing Date March 2019
Storage Conditions Room Temperature
Solvent/Matrix METHANOL

Certified Values

Analyte	Units	Certified Value ^{1,4}	Raw Material Purity,%	Analytical Value	Elution order	Raw Material Lot	CAS
2-FLUOROPHENOL	µg/mL	9930 ± 288	99.9	10037	1	LB92543	367-12-4
PHENOL-D6	µg/mL	9930 ± 290	99.4	9900	2	LB91168	13127-88-3
2,4,6-TRIBROMOPHENOL	µg/mL	9930 ± 318	99.7	9900	3	LB81262	118-79-6



Additional Information:

Analytical Method Parameters:

Column: SLB-5MS, 30 m x 0.25 mm x 0.25 µm df, Flow: 1.0 ml/min
Inlet: 200 °C, Injection Mode: Split, 60:1
80 °C (5 min) to 250 °C (3 min) at 40 °C/min
Detector: MSD, SIM, Transfer line: 250 °C
Injection Volume: 0.5 µL

ID #: 11383

Opened:

EPA 8270 Acids Surrogate Spike Mix HC

Expires: 3/31/2022

Rec'd: 4/10/2019

Energy Laboratories Inc 1120 So. 27th Street
Billings MT 59107



SIGMA-ALDRICH

2831 Soldier Springs Rd. Laramie, Wyoming 82070 USA
307-742-5452
rctechgroup@sigmaaldrich.com www.sigmaaldrich.com



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31086 **Lot No.:** A0166081

Description : B/N Surrogate Mix (4/89 SOW)
Base Neutral Surrogate 5000µg/mL, Methylene Chloride, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : October 31, 2026 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

ID #: 13328
Opened: _____
B/N Surrogate Mix (4/89 SOW)
Expires: 10/31/2026
Rec'd: 12/14/2020
Enerav Laboratories Inc 1120 So. 27th Street
Billings MT 59107

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)		
1	Nitrobenzene-d5 CAS # 4165-60-0 (Lot PR-29940B) Purity 99%	5,017.7 µg/mL	+/- 29.1731	µg/mL	Gravimetric
			+/- 225.9987	µg/mL	Unstressed
			+/- 250.7735	µg/mL	Stressed
2	2-Fluorobiphenyl CAS # 321-60-8 (Lot 00019169) Purity 99%	5,049.7 µg/mL	+/- 29.3592	µg/mL	Gravimetric
			+/- 227.4400	µg/mL	Unstressed
			+/- 252.3728	µg/mL	Stressed
3	p-Terphenyl-d14 CAS # 1718-51-0 (Lot PR-27278) Purity 99%	5,029.9 µg/mL	+/- 29.2444	µg/mL	Gravimetric
			+/- 226.5505	µg/mL	Unstressed
			+/- 251.3857	µg/mL	Stressed

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

Tech Tips:

Due to the limited solubility of p-terphenyl-d14 in methanol, we do not recommend that this mixture be diluted in methanol.

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

330°C

Det. Type:

FID

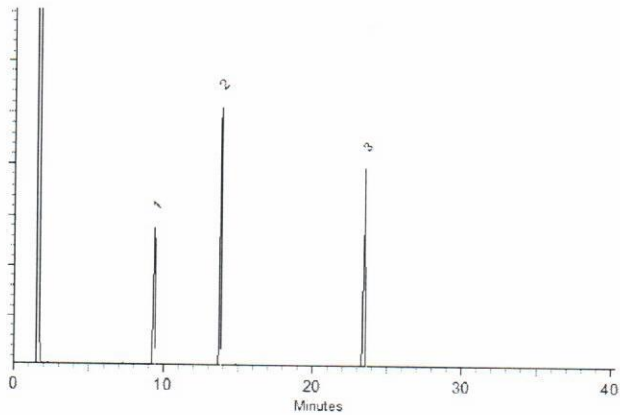

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Dalton Stover - Operations Technician I

Date Mixed: 04-Nov-2020

Balance: 1128353505

Justine Albertson - Operations Tech-ARM QC

Date Passed: 06-Nov-2020

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value (includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at www.restek.com/Contact-Us for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at www.restek.com/Contact-Us.
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.

ID #: 13510
 Opened: _____
 Dichloromethane EA342
Expires: 11/17/2022
 Rec'd: 1/26/2021
 Energy Laboratories Inc 1120 So 27th Street
 Billings MT 59107

Honeywell

CERTIFICATE OF ANALYSIS

Honeywell Burdick & Jackson®

1953 South Harvey Street
 Muskegon, MI 49442
 Phone: (800) 368-0050
 Fax: (231) 728-8226
lab.honeywell.com

Brand: Research Chemicals - B&J
Product: CS299AA-200
Lot No.: EA342
Production Date: 17-Nov-2020
Best Before: 17-Nov-2022

Dichloromethane, Custom, Contains Amylene Preservative, >99.9%
 for pesticide residue analysis

Parameter	Specification		Result	Units
	Min.	Max.		
Water by Karl Fischer Titration		0.010	0.0016	%
UV Cutoff		233	230	nm
Refractive Index (20°C)	1.4236	1.4246	1.4241	
Residue		1	<0.5	mg/L
GC Analysis	99.9		>99.99	%
Acidity (as HCl)		1	<1	mg/L
Chloride		10	<10	mg/L
Electron Capture GC		10	<10	ng/L
Flame Ionization GC		5	<5	ppb
UV Absorbance @ 240 nm		0.100	0.0920	AU
UV Absorbance @ 250 nm		0.010	0.0099	AU
UV Absorbance @ 300 nm		0.005	0.0008	AU
UV Absorbance @ 400 nm		0.005	0.0028	AU

**Honeywell
 Quality Control Approval**

Janna Dickinson

660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599
1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729
info@chemservice.com • www.chemservice.com

ID #: 13372

Opened:

Mixture #8-Internal Standards

Expires: 5/31/2022

Rec'd: 12/29/2020

Energy Laboratories Inc 1120 So. 27th Street
Billings MT 59107

CERTIFICATE OF ANALYSIS

Mixture #8-Internal Standards

CONCENTRATION 4000ug/ml in Methylene chloride
CATALOG NUMBER M-PPHC8X12-1ML
LOT NUMBER 10051700
DATE CERTIFIED 05/13/20
EXPIRATION DATE 05/31/22
STORAGE Store at room temperature (20 - 25 °C).
HANDLING See Safety Data Sheet
INTENDED USE For laboratory use only.
ISO 17034:2016 CERTIFIED [X]

ID	Analyte	CAS	Weight Analyte (mg)	Lot	Purity	Certified Concentration (ug/mL)
N-11000	Acenaphthene-d10	15067-26-2	1005.50	00027326	99.50	4001.9
N-11467	Chrysene-d12	1719-03-5	1012.20	00027327	98.80	4000.2
N-10217	1,4-Dichlorobenzene-d4	3855-82-1	1004.10	00027328	99.50	3996.3
N-12645	Naphthalene-d8	1146-65-2	1006.50	00025577	99.50	4005.9
N-12851	Perylene-d12	1520-96-3	1009.50	00027330	99.50	4017.8
N-12856	Phenanthrene-d10	1517-22-2	1021.10	00027331	99.00	4043.6

Analytical Test

CONCENTRATION (GC/FID)

Value

VERIFIED

Instructions for Use:

Shake mixture prior to use. If particles are present, sonicate for homogeneity. If sample is diluted to lower concentrations, Class A volumetric glassware must be used.

Minimum Sample Size- 0.2 uL for Direct Injection.

Chem Service Inc. guarantees the expanded uncertainty of the above analytes to be +/- 2.0% of the certified concentrations based on gravimetric preparation. The test results published in this report were obtained using equipment capable of producing results that are traceable to NIST and through NIST to the International System of Units (SI). The reported expanded uncertainty of measurement is stated as the combined standard uncertainty of measurement multiplied by the coverage factor k (k=2) such that the coverage probability corresponds to approximately 95%. For certified reference materials, homogeneity and thermal stability testing are available upon request.

Certified By:

Mary Beth O'Donnell

Mary Beth O'Donnell
CSM/TC

Chem Service is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015



COA Form
Revision 3 (3/2015)


660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599
 1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729
info@chemservice.com • www.chemservice.com

Gas

Data file: C:\CHEM3\
 Sample name: M-PPCH8X
 Instrument: GC 2
 Injection date: 5/13/2020 8:56:25 AM
 Acq. method: M-PPHC8X12.M
 Column name: HP-5

CERTIFICATE OF ANALYSIS

Sample type: Sample
 Location: Vial 3
 Injection volume: 1.0uL



Signal: FID1 A, Front Signal

RT [min]	Type	Width [min]	Area	Height	Area%
5.427	BB	0.0181	1240.1130	1041.0874	8.36
6.593	BB	0.0189	2274.8877	1876.2654	15.33
8.272	BB	0.0196	2371.0022	1888.8049	15.98
9.696	BV	0.0197	2694.9399	2106.0442	18.16
12.654	BB	0.0330	2999.0918	1397.3110	20.21
16.001	BB	0.0562	3260.5679	751.0330	21.97
		Sum	14840.6025		

Chem Service is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015





CERTIFIED WEIGHT REPORT

Part Number: 92180
Lot Number: 020221
Description: CLP Semi-Volatile Calibration Standard
64 components
Expiration Date: 020228
Recommended Storage: Freezer (0 °C)
Nominal Concentration (µg/mL): 1000
NIST Test ID#: 23060

Solvent: Methylene chloride
Lot#: 104929

Eli Aliaga 020221
Formulated By: **Eli Aliaga** DATE
Pedro L. Rentas 020221
Reviewed By: **Pedro L. Rentas** DATE

Weight(s) shown below were combined and diluted to (mL): 100.0 0.003 Balance Uncertainty 5E-05 Flask Uncertainty

Compound	(RM#) Part Number	Lot Number	Dil. Factor	Initial Vol. (mL)	Initial Conc. (µg/mL)	Nominal Conc. (µg/mL)	Purity (%)	Uncertainty Purity (%)	Uncertainty Pipette (mL)	Target Weight (g)	Actual Weight (g)	Actual Conc. (µg/mL)	Expanded Uncertainty (Solvent Safety Info. On Attached pg.)			
													(+/-) (µg/mL)	CAS#	OSHA PEL (TWA) L50	
1. 2,2'-Oxybis(1-chloropropane)	(0078)	012016AR	NA	NA	NA	1000	98.9	0.2	NA	0.10112	0.10135	1002.3	4.2	108-60-1	N/A	ori-rat 240mg/kg
2. Hexachlorobenzene	(0195)	051897	NA	NA	NA	1000	99	0.2	NA	0.10102	0.10121	1001.9	4.2	118-74-1	N/A	ori-rat 10g/kg
3. bis(2-Chloroethoxy) methane	10111	011214	0.05	5.00	20018.4	1000	NA	NA	0.017	NA	NA	1000.8	8.0	111-91-1	N/A	N/A
4. bis(2-Chloroethyl) ether	10111	011214	0.05	5.00	20012.4	1000	NA	NA	0.017	NA	NA	1000.5	8.0	111-44-4	15 ppm (90mg/m3/8H)(skin)	ori-rat 75mg/kg
5. bis(2-Ethylhexyl) phthalate	10111	011214	0.05	5.00	20014.3	1000	NA	NA	0.017	NA	NA	1000.6	8.0	117-81-7	5mg/m3/8H	ori-rat 3060mg/kg
6. 4-Bromophenyl phenyl ether	10111	011214	0.05	5.00	20008.8	1000	NA	NA	0.017	NA	NA	1000.3	8.0	101-55-3	N/A	N/A
7. Benzyl butyl phthalate	10111	011214	0.05	5.00	20011.3	1000	NA	NA	0.017	NA	NA	1000.5	8.0	85-68-7	N/A	ori-rat 2330mg/kg
8. 4-Chlorophenyl phenyl ether	10111	011214	0.05	5.00	20009.5	1000	NA	NA	0.017	NA	NA	1000.4	8.0	7005-72-3	N/A	N/A
9. Diethyl phthalate	10111	011214	0.05	5.00	20013.6	1000	NA	NA	0.017	NA	NA	1000.6	8.0	84-66-2	5mg/m3/8H	ori-rat 8600mg/kg
10. Dimethyl phthalate	10111	011214	0.05	5.00	20015.7	1000	NA	NA	0.017	NA	NA	1000.7	8.0	131-11-3	5mg/m3/8H	ori-rat 6800mg/kg
11. Di-n-butyl phthalate	10111	011214	0.05	5.00	20011.6	1000	NA	NA	0.017	NA	NA	1000.5	8.0	84-74-2	5mg/m3/8H	ori-rat 8000mg/kg
12. Di-n-octyl phthalate	10111	011214	0.05	5.00	20012.2	1000	NA	NA	0.017	NA	NA	1000.5	8.0	117-84-0	N/A	ori-rat 4700mg/kg
13. N-Nitrosodimethylamine	10111	011214	0.05	5.00	20010.0	1000	NA	NA	0.017	NA	NA	1000.4	8.0	62-75-9	N/A	ori-rat 58mg/kg
14. N-Nitrosodi-n-propylamine	10111	011214	0.05	5.00	20010.5	1000	NA	NA	0.017	NA	NA	1000.4	8.0	621-64-7	N/A	ori-rat 460mg/kg
15. 1,2-Diphenylhydrazine (as Azobenzene)	10112	042820	0.05	5.00	20003.9	1000	NA	NA	0.017	NA	NA	1000.1	8.1	103-33-3	N/A	ori-rat 1000mg/kg
16. 2-Chloronaphthalene	10112	042820	0.05	5.00	20002.3	1000	NA	NA	0.017	NA	NA	1000.0	8.0	91-58-7	N/A	ori-rat 2078mg/kg
17. 1,2-Dichlorobenzene	10112	042820	0.05	5.00	20005.4	1000	NA	NA	0.017	NA	NA	1000.2	8.0	95-50-1	50 ppm (300mg/m3) (CL)	ori-rat 500mg/kg
18. 1,3-Dichlorobenzene	10112	042820	0.05	5.00	20007.7	1000	NA	NA	0.017	NA	NA	1000.1	8.0	541-73-1	N/A	ipr-mus 1062mg/kg
19. 1,4-Dichlorobenzene	10112	042820	0.05	5.00	20005.4	1000	NA	NA	0.017	NA	NA	1000.2	8.0	108-46-7	75 ppm (450mg/m3/8H)	ori-rat 500mg/kg
20. 2,4-Dinitrotoluene	10112	042820	0.05	5.00	20003.3	1000	NA	NA	0.017	NA	NA	1000.1	8.1	121-14-2	1.5mg/m3/8H (skin)	ori-rat 268mg/kg
21. 2,6-Dinitrotoluene	10112	042820	0.05	5.00	20002.4	1000	NA	NA	0.017	NA	NA	1000.0	8.0	606-20-2	1.5mg/m3/8H (skin)	ori-rat 177mg/kg
22. Hexachloro-1,3-butadiene	10112	042820	0.05	5.00	20009.4	1000	NA	NA	0.017	NA	NA	1000.4	12.4	87-68-3	0.02 ppm (0.24mg/m3/8H)	ori-rat 82mg/kg
23. Hexachlorocyclopentadiene	10112	042820	0.05	5.00	20001.8	1000	NA	NA	0.017	NA	NA	1000.0	8.0	77-47-4	0.01 ppm (0.1mg/m3/8H)	ori-rat 1300mg/kg
24. Hexachloroethane	10112	042820	0.05	5.00	20002.4	1000	NA	NA	0.017	NA	NA	1000.0	8.0	67-72-1	1 ppm (10mg/m3/8H)(skin)	ori-ggq 4070mg/kg
25. Isophorone	10112	042820	0.05	5.00	20003.8	1000	NA	NA	0.017	NA	NA	1000.1	8.1	78-59-1	25 ppm	ori-rat 2330mg/kg
26. Nitrobenzene	10112	042820	0.05	5.00	20004.9	1000	NA	NA	0.017	NA	NA	1000.1	8.0	98-95-3	1 ppm (8mg/m3/8H)(skin)	ori-rat 780mg/kg
27. 1,2,4-Trichlorobenzene	10112	042820	0.05	5.00	20002.0	1000	NA	NA	0.017	NA	NA	1000.0	8.0	120-82-1	5 ppm (CL) (40mg/m3)	ori-rat 758mg/kg
28. o-Cresol (2-Methylphenol)	10114	081919	0.05	5.00	20010.2	1000	NA	NA	0.017	NA	NA	1000.4	8.0	95-48-7	5 ppm (22mg/m3/8H)(skin)	ori-rat 121mg/kg
29. p-Cresol (4-Methylphenol)	10114	081919	0.05	5.00	20061.2	1000	NA	NA	0.017	NA	NA	1003.0	8.0	106-44-5	5 ppm (22mg/m3/8H)(skin)	ori-rat 207mg/kg
30. 2,4,5-Trichlorophenol	10114	081919	0.05	5.00	20023.2	1000	NA	NA	0.017	NA	NA	1001.1	8.0	95-95-4	N/A	ori-rat 820mg/kg
31. 4-Chloroaniline	10115	080512	0.05	5.00	20009.6	1000	NA	NA	0.017	NA	NA	1000.4	8.0	106-47-8	N/A	ori-rat 310mg/kg
32. Dibenzofuran	10115	080512	0.05	5.00	20020.2	1000	NA	NA	0.017	NA	NA	1000.9	8.0	132-64-9	N/A	N/A
33. 2-Methylnaphthalene	10115	080512	0.05	5.00	20012.9	1000	NA	NA	0.017	NA	NA	1000.5	8.1	91-57-6	N/A	ori-rat 1630mg/kg
34. 2-Nitroaniline	10115	080512	0.05	5.00	20011.8	1000	NA	NA	0.017	NA	NA	1000.5	8.0	88-74-4	N/A	ori-rat 1600mg/kg
35. 3-Nitroaniline	10115	080512	0.05	5.00	20018.6	1000	NA	NA	0.017	NA	NA	1000.8	8.0	99-09-2	N/A	ori-rat 535mg/kg
36. 4-Nitroaniline	10115	080512	0.05	5.00	20014.9	1000	NA	NA	0.017	NA	NA	1000.6	8.0	100-01-6	1 ppm (8mg/m3/8H)(skin)	ori-rat 750mg/kg
37. 4-Chloro-3-methylphenol	10118	072120	0.05	5.00	20003.9	1000	NA	NA	0.017	NA	NA	1000.1	8.0	59-50-7	N/A	ori-rat 1830mg/kg
38. 2-Chlorophenol	10118	072120	0.05	5.00	20002.9	1000	NA	NA	0.017	NA	NA	1000.0	8.0	95-57-8	N/A	ori-rat 670mg/kg
39. 2,4-Dichlorophenol	10118	072120	0.05	5.00	20003.1	1000	NA	NA	0.017	NA	NA	1000.1	8.0	120-83-2	N/A	ori-rat 580mg/kg
40. 2,4-Dimethylphenol	10118	072120	0.05	5.00	20003.3	1000	NA	NA	0.017	NA	NA	1000.1	8.1	105-67-9	N/A	ori-rat 3200mg/kg
41. 2,4-Dinitrophenol	10118	072120	0.05	5.00	20001.8	1000	NA	NA	0.017	NA	NA	1000.0	8.0	51-28-5	N/A	ori-rat 30mg/kg
42. 4,6-Dinitro-2-methylphenol	10118	072120	0.05	5.00	20002.5	1000	NA	NA	0.017	NA	NA	1000.0	8.0	534-52-1	N/A	N/A
43. 2-Nitrophenol	10118	072120	0.05	5.00	20003.7	1000	NA	NA	0.017	NA	NA	1000.1	8.0	88-75-5	N/A	ori-rat 334mg/kg
44. 4-Nitrophenol	10118	072120	0.05	5.00	20002.0	1000	NA	NA	0.017	NA	NA	1000.0	8.0	100-02-7	N/A	ori-rat 250mg/kg
45. Pentachlorophenol	10118	072120	0.05	5.00	20002.8	1000	NA	NA	0.017	NA	NA	1000.0	8.0	87-86-5	0.5mg/m3/8H (skin)	ori-rat 27mg/kg
46. Phenol	10118	072120	0.05	5.00	20003.9	1000	NA	NA	0.017	NA	NA	1000.1	8.0	108-95-2	5 ppm (18mg/m3/8H)(skin)	ori-rat 317mg/kg
47. 2,4,6-Trichlorophenol	10118	072120	0.05	5.00	20004.2	1000	NA	NA	0.017	NA	NA	1000.1	8.0	88-06-2	N/A	ori-rat 820mg/kg
48. Acenaphthene	10007	042420	0.50	50.00	2001.2	1000	NA	NA	0.018	NA	NA	1000.5	4.1	83-32-9	N/A	ipr-rat 600mg/kg
49. Acenaphthylene	10007	042420	0.50	50.00	2000.2	1000	NA	NA	0.018	NA	NA	1000.0	4.2	208-96-8	N/A	N/A
50. Anthracene	10007	042420	0.50	50.00	2000.3	1000	NA	NA	0.018	NA	NA	1000.1	4.1	120-12-7	0.2mg/m3 (8H)	ipr-mus 430mg/kg
51. Benzo(a)anthracene	10007	042420	0.50	50.00	2001.3	1000	NA	NA	0.018	NA	NA	1000.6	4.2	56-55-3	N/A	N/A
52. Benzo(a)pyrene	10007	042420	0.50	50.00	2000.0	1000	NA	NA	0.018	NA	NA	999.9	4.1	50-32-8	0.2mg/m3 (8H)	scu-rat 50mg/kg
53. Benzo(b)fluoranthene	10007	042420	0.50	50.00	2000.9	1000	NA	NA	0.018	NA	NA	1000.4	4.1	205-99-2	N/A	N/A
54. Benzo(k)fluoranthene	10007	042420	0.50	50.00	2001.2	1000	NA	NA	0.018	NA	NA	1000.5	4.1	207-08-9	N/A	N/A
55. Benzo(g,h,i)perylene	10007	042420	0.50	50.00	2000.0	1000	NA	NA	0.018	NA	NA	999.9	4.1	191-24-2	N/A	N/A
56. Carbazole	10007	042420	0.50	50.00	2000.3	1000	NA	NA	0.018	NA	NA	1000.0	4.2	86-74-8	N/A	ipr-mus 200mg/kg
57. Chrysene	10007	042420	0.50	50.00	2000.8	1000	NA	NA	0.018	NA	NA	1000.3	4.2	218-01-9	0.2mg/m3	N/A
58. Dibenzo(a,h)anthracene	10007	042420	0.50	50.00	2000.8	1000	NA	NA	0.018	NA	NA	1000.3	4.2	53-70-3	0.2mg/m3	N/A
59. Fluoranthene	10007	042420	0.50	50.00	2000.3	1000	NA	NA	0.018	NA	NA	1000.1	4.2	206-44-0	N/A	ori-rat 2000mg/kg
60. Fluorene	10007	042420	0.50	50.00	2000.9	1000	NA	NA	0.018	NA	NA	1000.3	4.2	86-73-7	N/A	ipr-mus 2 g/kg
61. Indeno(1,2,3-cd)pyrene	10007	042420	0.50	50.00	2000.1	1000	NA	NA	0.018	NA	NA	1000.0	4.1	193-39-5	N/A	N/A
62. Naphthalene	10007	042420	0.50	50.00	2000.9	1000	NA	NA	0.018	NA	NA	1000.4	4.1	91-20-3	10 ppm (50mg/m3/8H)	ori-rat 480mg/kg
63. Phenanthrene	10007	042420	0.50	50.00	2000.9	1000	NA	NA	0.018	NA	NA	1000.4	4.1	85-01-8	0.2mg/m3/8H	ori-mus 700mg/kg
64. Pyrene	10007	042420	0.50	50.00	2001.0	1000	NA	NA	0.018	NA	NA	1000.4	4.2	129-00-0	0.2mg/m3/8H	ori-rat 2700mg/kg


* The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
* Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
* Standards are certified (±) 0.5% of the stated value, unless otherwise stated.
* All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
* Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

ID #: 13539

Opened: _____
CLP Semi-Volatile Calibration Standard
Expires: 2/2/2026
Rec'd: 2/5/2021
Energy Laboratories Inc 1120 So. 27th Street
Billings MT 59107



Method GC8MSD-2.M: Column:SBB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (14 min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 290°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by Melissa Stonier.

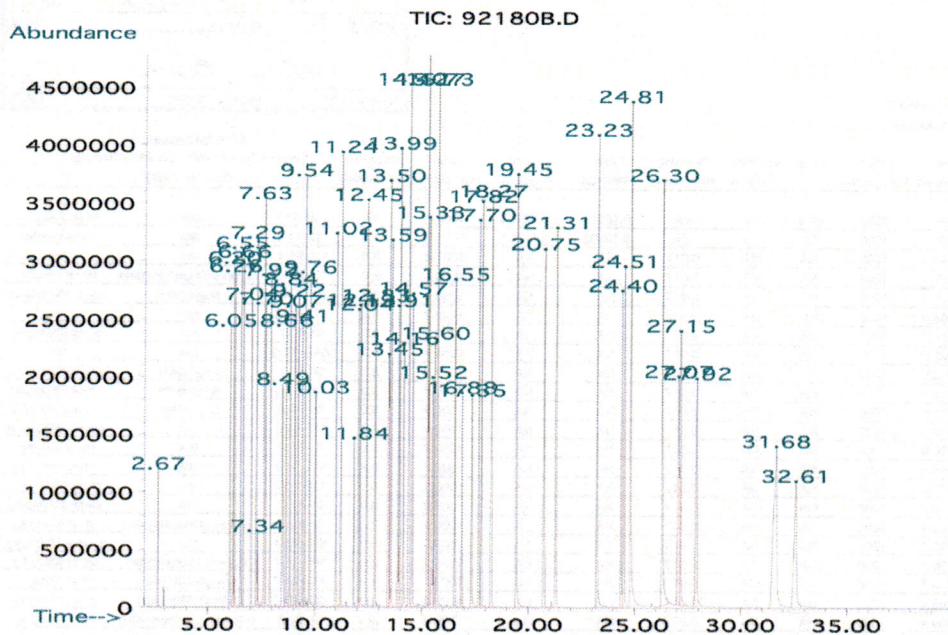

Peak No	Name	MSD RT (min.)
1	N-nitrosodimethylamine	2.67
2	Phenol	6.05
3	bis(2-Chloroethyl)ether	6.20
4	2-Chlorophenol	6.26
5	1,3-Dichlorobenzene	6.55
6	1,4-Dichlorobenzene	6.63
7	1,2-Dichlorobenzene	7.04
8	o-Cresol (2-methylphenol)	7.29
9	bis(2-Chloroisopropyl)ether	7.34
10	p-Cresol (4-methylphenol)/N-nitrosodi-n-propylamine	7.63
11	Hexachloroethane	7.70
12	Nitrobenzene	7.92
13	Isophorone	8.49
14	2-Nitrophenol	8.66
15	2,4-Dimethylphenol	8.84
16	bis(2-Chloroethoxy)methane	9.07
17	2,4-Dichlorophenol	9.22
18	1,2,4-Trichlorobenzene	9.41
19	Naphthalene	9.54
20	4-Chloroaniline	9.76
21	Hexachloro-1,3-butadiene	10.03
22	4-Chloro-3-methylphenol	11.02
23	2-Methylnaphthalene	11.24
24	Hexachlorocyclopentadiene	11.84
25	2,4,6-Trichlorophenol	12.04
26	2,4,5-Trichlorophenol	12.13
27	2-Chloronaphthalene	12.45
28	2-Nitroaniline	12.84
29	Dimethyl phthalate	13.45
30	Acenaphthylene	13.50
31	2,6-Dinitrotoluene	13.59
32	3-Nitroaniline	13.91
33	Acenaphthene	13.99
34	2,4-Dinitrophenol	14.16
35	Dibenzofuran/4-Nitrophenol	14.40
36	2,4-Dinitrotoluene	14.57
37	Diethyl phthalate/Fluorene	15.27
38	4-Chlorophenyl phenyl ether	15.33
39	4-Nitroaniline	15.52
40	4,6-Dinitro-2-methylphenol	15.60
41	Azobenzene	15.73
42	4-Bromophenyl phenyl ether	16.56
43	Hexachlorobenzene	16.89
44	Pentachlorophenol	13.35
45	Phenanthrene	17.70
46	Anthracene	17.82
47	Carbazole	18.27
48	Di-n-butyl phthalate	19.45
49	Fluoranthene	20.75
50	Pyrene	21.31
51	Benzyl butyl phthalate	23.23
52	Benzo(a)anthracene	24.40
53	Chrysene	24.51
54	bis(2-Ethylhexyl)phthalate	24.82
55	Di-n-octyl phthalate	26.30
56	Benzo(b)fluoranthene	27.07
57	Benzo(k)fluoranthene	27.15
58	Benzo(a)pyrene	27.92
59	Indeno(1,2,3-cd)pyrene/Dibenzo(a,h)anthracene	31.68
60	Benzo(g,h,i)perylene	32.61



Analytical RunID SV5975.I_220207A Standards Traceability Report

Spike ID: sv100418

Spike Name: BNA mix 200 ug/mL

Prep Date: 6/2/2021

Exp Date: 3/31/2022

Department: GCMSSEMI

Vendor:

Lot Number:

Balance ID:

Comments:

Type: Secondary

Prep By: John P. Heine

Status: New

Final Volume: 1.5 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Dichloromethane EA342	13510	0.51	mL	3/31/2022

Stock Source	Base Units	Amount Added
sv82908	ug/mL	0.03 mL
sv83301	ug/mL	0.15 mL
sv83120	ug/mL	0.15 mL
sv83419	ug/mL	0.15 mL
sv82917	ug/mL	0.15 mL
sv83410	ug/mL	0.15 mL
sv83407	ug/mL	0.06 mL
sv83201	ug/mL	0.15 mL



Analytical RunID SV5975.I_220207A Standards Traceability Report

Spike ID: sv100506

Spike Name: BNA low 50 ug/mL

Prep Date: 6/2/2021

Exp Date: 3/31/2022

Department: GCMSSEMI

Vendor:

Lot Number:

Balance ID:

Comments:

Type: Secondary

Prep By: John P. Heine

Status: New

Final Volume: 0.8 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Dichloromethane EA342	13510	0.6	mL	3/31/2022

Stock Source	Base Units	Amount Added
sv100418	ug/mL	0.2 mL



Analytical RunID SV5975.I_220207A Standards Traceability Report

Spike ID: sv100703

Spike Name: BNA Internals 2000 ug/mL

Prep Date: 12/9/2021

Exp Date: 5/31/2022

Department: GCMSSEMI

Vendor: Chemservice

Lot Number: 8443500

Balance ID:

Comments:

Type: Secondary

Prep By: John P. Heine

Status: New

Final Volume: 2.12 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Dichloromethane EA342	13510	1.06	mL	5/31/2022

Stock Source	Base Units	Amount Added
sv83403	ug/mL	1.06 mL



Analytical RunID SV5975.I_220207A Standards Traceability Report

Spike ID: sv100801

Spike Name: BNA 2nd source 200ug/mL

Prep Date: 1/17/2022

Exp Date: 10/1/2022

Department: GCMSSEMI

Vendor:

Lot Number:

Balance ID:

Comments:

Type: Secondary

Prep By: John P. Heine

Status: New

Final Volume: 1 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Dichloromethane EA342	13510	540	uL	10/1/2022

Stock Source	Base Units	Amount Added
sv83514	ug/mL	0.1 mL
sv82702	ug/mL	0.02 mL
sv83218	ug/mL	0.1 mL
sv83512	ug/mL	0.2 mL
sv83411	ug/mL	0.04 mL



Analytical RunID SV5975.I_220207A Standards Traceability Report

Standard ID: sv82702

Standard Name: AE Surr

Prep Date: 8/28/2018

Exp Date: 4/30/2023

Department: GCMSPR

Vendor: Restek

Lot Number: A0137474

Balance ID:

Comments:

Type: Primary

Prep By: Craig A. Bardelli

Status: New

Final Volume: mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Acid Surrogate Standard Mix (4/89)	10707	1	mL	4/30/2023
Stock Source	Base Units	Amount Added		



Analytical RunID SV5975.I_220207A Standards Traceability Report

Spike ID: sv82908

Spike Name: AE surr

Prep Date: 4/10/2019

Exp Date: 3/31/2022

Department: GCMSSEMI

Vendor: Sigma-Aldrich

Lot Number: LRAC2239

Balance ID:

Comments:

Type: Primary

Prep By: Sean McGrew

Status: New

Final Volume: mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
EPA 8270 Acids Surrogate Spike Mix HC	11383		mL	3/31/2022
Stock Source	Base Units	Amount Added		



Analytical RunID SV5975.I_220207A Standards Traceability Report

Spike ID: sv82917

Spike Name: BNA Custom for Cal

Prep Date: 6/3/2019

Exp Date: 5/28/2023

Department: GCMSSEMI

Vendor: AccuStandard

Lot Number: 219051432

Balance ID:

Comments: Date prepared is date received (10 1mL ampules) - recert from 6/21/21 to 5/28/23

Type: Primary

Prep By: John P. Heine

Status: New

Final Volume: 1 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Custom BNA Mix	11547	1	mL	5/28/2023

Stock Source	Base Units	Amount Added
--------------	------------	--------------



Analytical RunID SV5975.I_220207A Standards Traceability Report

Spike ID: sv83120

Spike Name: BN mix

Prep Date: 3/12/2020

Exp Date: 1/31/2023

Department: GCMSSEMI

Vendor: Sigma-Aldrich

Lot Number: LRAC4915

Balance ID:

Comments:

Type: Primary

Prep By: Sean McGrew

Status: New

Final Volume: 1 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
TCL Base-Neutrals Mix	12503	1	mL	1/31/2023

Stock Source	Base Units	Amount Added
--------------	------------	--------------



Analytical RunID SV5975.I_220207A Standards Traceability Report

Spike ID: sv83201

Spike Name: Phenols mix

Prep Date: 3/17/2020

Exp Date: 1/31/2028

Department: GCMSSEMI

Vendor: Restek

Lot Number: A0157111

Balance ID:

Comments:

Type: Primary

Prep By: Sean McGrew

Status: New

Final Volume: 1 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
604 Phenols Calibration Mix	12512		mL	1/31/2028
Stock Source	Base Units	Amount Added		



Analytical RunID SV5975.I_220207A Standards Traceability Report

Spike ID: sv83218

Spike Name: Benzidines

Prep Date: 7/7/2020

Exp Date: 5/1/2024

Department: GCMSSEMI

Vendor: AccuStandard

Lot Number: 220041353

Balance ID:

Comments: 2000 ug/mL 12839

Type: Primary

Prep By: John P. Heine

Status: New

Final Volume: 1 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Benzidine & 3,3'-Dichlorobenzidine	12839	1	mL	5/1/2024

Stock Source	Base Units	Amount Added
--------------	------------	--------------



Analytical RunID SV5975.I_220207A Standards Traceability Report

Spike ID: sv83301

Spike Name: PAH Mix

Prep Date: 7/13/2020

Exp Date: 9/30/2022

Department: GCMSSEMI

Vendor: Sigma-Aldrich

Lot Number: LRAC3877

Balance ID:

Comments: 4 x 1mL

Type: Primary

Prep By: John P. Heine

Status: New

Final Volume: 6 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
TCL PAH Mix	12846	6	mL	9/30/2022
Stock Source	Base Units	Amount Added		



Analytical RunID SV5975.I_220207A Standards Traceability Report

Spike ID: sv83403

Spike Name: BNA Internals 4000ug/mL

Prep Date: 12/29/2020

Exp Date: 5/31/2022

Department: GCMSSEMI

Vendor: Chemservice

Lot Number: 10051700

Balance ID:

Comments:

Type: Primary

Prep By: John P. Heine

Status: New

Final Volume: 8 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Mixture #8-Internal Standards	13372	8	mL	5/31/2022
Stock Source	Base Units	Amount Added		



Analytical RunID SV5975.I_220207A Standards Traceability Report

Standard ID: sv83407

Standard Name: BN Surr 5000 ug/mL

Prep Date: 12/14/2020

Exp Date: 10/31/2026

Department: GCMSSEMI

Vendor: Restek

Lot Number: A0166081

Balance ID:

Comments:

Type: Primary

Prep By: John P. Heine

Status: New

Final Volume: 5 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
B/N Surrogate Mix (4/89 SOW)	13328	1	mL	10/31/2026

Stock Source	Base Units	Amount Added
--------------	------------	--------------



Analytical RunID SV5975.I_220207A Standards Traceability Report

Spike ID: sv83410

Spike Name: H.S. Mix

Prep Date: 4/7/2021

Exp Date: 2/28/2024

Department: GCMSSEMI

Vendor: Sigma-Aldrich

Lot Number: LRAC9004

Balance ID:

Comments: 2000 ug/mL

Type: Primary

Prep By: Sean McGrew

Status: New

Final Volume: mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
EPA TCL Hazardous Substances Mix (12 cmpds)	13691		mL	2/28/2024

Stock Source	Base Units	Amount Added
--------------	------------	--------------



Analytical RunID SV5975.I_220207A Standards Traceability Report

Spike ID: sv83411

Spike Name: BN surr

Prep Date: 4/7/2021

Exp Date: 11/20/2026

Department: GCMSSEMI

Vendor: Restek

Lot Number: A6167670

Balance ID:

Comments: 5000 ug/mL

Type: Primary

Prep By: Sean McGrew

Status: New

Final Volume: mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
B/N Surrogate Mix (4/89 SOW)	13666		mL	11/20/2026
Stock Source	Base Units	Amount Added		



Analytical RunID SV5975.I_220207A Standards Traceability Report

Spike ID: sv83419

Spike Name: Benzidines CAL 2000ug/mL

Prep Date: 5/18/2021

Exp Date: 4/30/2023

Department: GCMSSEMI

Vendor: Agilent

Lot Number: 0006592783

Balance ID:

Comments: 2000 ug/mL

Type: Primary

Prep By: John P. Heine

Status: New

Final Volume: 1 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Benzidines Standard	13854	1	mL	4/30/2023
Stock Source	Base Units	Amount Added		



Analytical RunID SV5975.I_220207A Standards Traceability Report

Spike ID: sv83512

Spike Name: 625 LCS Spk

Prep Date: 7/30/2021

Exp Date: 2/2/2026

Department: GCMSPR

Vendor: Absolute Standards

Lot Number: 020221

Balance ID:

Comments: 12x1mL ampules

Type: Primary

Prep By: Ryan F. Bengel

Status: Open

Final Volume: 1 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
CLP Semivolatile Calibration Standard	14074	1	mL	2/2/2026
Stock Source	Base Units	Amount Added		



Analytical RunID SV5975.I_220207A Standards Traceability Report

Spike ID: sv83514

Spike Name: Additional

Prep Date: 9/22/2021

Exp Date: 10/1/2022

Department: GCMSPR

Vendor: AccuStandard

Lot Number: 22002155-02

Balance ID:

Comments: 12x1mL ampules

Type: Primary

Prep By: Ryan F. Bengel

Status: Open

Final Volume: 1 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Custom Semi-Volatile Standard	14279	1	mL	10/1/2022

Stock Source	Base Units	Amount Added
--------------	------------	--------------



110 Benner Circle
 Bellefonte, PA 16823-8812
 Tel: (800)356-1688
 Fax: (814)353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31063 Lot No.: A0137474
 Description : Acid Surrogate Standard Mix (4/89)
Acid Surrogate Standard Mix (4/89) 10,000 µg/mL, Methanol, 1mL/ampul
 Container Size : 2 mL Pkg Amt: > 1 mL
 Expiration Date : April 30, 2023 Storage: 10°C or colder

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L., K=2)
1	2-Fluorophenol	10,046.4 µg/mL	+/- 58.8239 µg/mL
	CAS # 367-12-4 (Lot STBD7945V)		+/- 293.2702 µg/mL
	Purity 99%		+/- 355.8400 µg/mL
2	Phenol-d6	10,023.6 µg/mL	+/- 58.6904 µg/mL
	CAS # 13127-88-3 (Lot PR-27801)		+/- 292.6047 µg/mL
	Purity 99%		+/- 355.0324 µg/mL
3	2,4,6-Tribromophenol	10,057.2 µg/mL	+/- 58.8871 µg/mL
	CAS # 118-79-6 (Lot 29699MJV)		+/- 293.5855 µg/mL
	Purity 99%		+/- 356.2225 µg/mL

Solvent: Methanol
 CAS # 67-56-1
 Purity 99%

ID #: 10707
 Opened: _____
 Acid Surrogate Standard Mix (4/89)
 Expires: 4/30/2023
 Rec'd: 8/24/2018
 Energy Laboratories Inc 1120 So 27th Street
 Billings MT 59107

Certificate of Analysis

EPA 8270 ACIDS SURROGATE SPIKE MIX
HC,1X1ML,10MG/ML,METHANOL


*Certified
Reference
Material*

Description

Product ID 47260-U
Lot LRAC2239
Expiration Date March 2022
Manufacturing Date March 2019
Storage Conditions Room Temperature
Solvent/Matrix METHANOL

Certified Values

Analyte	Units	Certified Value ^{1,4}	Raw Material Purity,%	Analytical Value	Elution order	Raw Material Lot	CAS
2-FLUOROPHENOL	µg/mL	9930 ± 288	99.9	10037	1	LB92543	367-12-4
PHENOL-D6	µg/mL	9930 ± 290	99.4	9900	2	LB91168	13127-88-3
2,4,6-TRIBROMOPHENOL	µg/mL	9930 ± 318	99.7	9900	3	LB81262	118-79-6



Additional Information:

Analytical Method Parameters:

Column: SLB-5MS, 30 m x 0.25 mm x 0.25 µm df , Flow: 1.0 ml/min
Inlet: 200 °C, Injection Mode: Split, 60:1
80 °C (5 min) to 250 °C (3 min) at 40 °C /min
Detector: MSD, SIM, Transfer line: 250 °C
Injection Volume: 0.5 µL

ID #: 11383

Opened:

EPA 8270 Acids Surrogate Spike Mix HC

Expires: 3/31/2022

Rec'd: 4/10/2019

Enerav Laboratories Inc 1120 So. 27th Street
Billings MT 59107



SIGMA-ALDRICH®

2931 Soldier Springs Rd. Laramie, Wyoming 82070 USA
307-742-5452
rctechgroup@sia.com www.sigma-aldrich.com

CERTIFICATE OF ANALYSIS

Catalog No: S-6237A-R1

Description: Custom BNA Mix

Lot: 219051432-01

Solvent: Dichloromethane

Hazards: Refer to SDS for complete safety information

Date Certified: Apr 28, 2021

Expiration: May 28, 2023

Sample Size: 1 mL


Components: 6

Storage Condition: Ambient (>5 °C)



Signal Word: Warning

Certified Reference Material



Component	CAS #	Purity %	Prepared Concentration ²	Certified Analyte Concentration ¹
		(GC/MS)	(µg/mL)	(µg/mL)
4-Chloro-2-methylphenol	1570-64-5	97.0	2064*	2002
4-Chlorophenol	106-48-9	98.6	2012	1984
1-Methylnaphthalene	90-12-0	99.7	2016	2010
Pyridine	110-86-1	98.7	2003	1977
o-Terphenyl	84-15-1	99.9	2003	2001
Triallate	2303-17-5	99.9	2013	2011

ID #: 11547

Opened: _____

Custom BNA Mix

Expires: 5/28/2023

Rec'd: 5/31/2019

Enerav Laboratories Inc 1120 So. 27th Street
Billings MT 59107

* Weight compensated to 100% purity.

A product with a suffix (-1A, -2B, etc. or -01, -02, etc.) on its lot number has had its expiration date extended and is identical to the same lot number without the suffix.

² All weights are traceable through NIST, Test No. 684/289871-17

¹ Certified Analyte Concentration = Purity x Prepared Concentration.

The Uncertainty associated with the certified concentration reported on this certificate is ±2.4%. This value is the combined expanded uncertainty and represents an estimated standard deviation equal to the positive square root of the total variation of the uncertainty of components. A normal distribution is assumed and a coverage factor of K=2 is chosen using approximately a 95% confidence level.

Labels and certificates follow U.S. Conventions in reporting numerical values: A comma (,) is used to separate units of one-thousand or greater. A period (.) is used as a decimal place marker.

The information on this certificate may not be reproduced without the express permission of the manufacturer. See reverse side for additional information

Hazard Information: Please refer to the SDS for information regarding the hazards associated with using this material.

This product was prepared according to in-house procedures and is guaranteed to be homogeneous.

Certified By: _____

Larry Decker, Organic QC Manager

Certificate of Analysis

TCL BASE-NEUTRALS
MIX, 1X1 ML, 2000 UG/ML, DICHLOROMETHANE

Certified
Reference
Material

Description

Product ID 47991-U
Lot LRAC4915
Expiration Date January 2023
Manufacturing Date January 2020
Storage Conditions Refrigerate
Solvent/Matrix DICHLOROMETHANE

Certified Values

Analyte	Certified Value ^{1,4}	Units	Raw Material Purity, %	Elution order	Raw Material Lot	CAS
N-NITROSODIMETHYLAMINE	1999 ± 39	µg/mL	98.1	1	11-RFS-142-1	62-75-9
BIS (2-CHLOROETHYL) ETHER	2003 ± 42	µg/mL	99.4	2	06413MS	111-44-4
1,3-DICHLOROBENZENE	2001 ± 47	µg/mL	99.6	3	11221HC	541-73-1
1,4-DICHLOROBENZENE	2000 ± 66	µg/mL	99.9	4	MKBG7690V	106-46-7
1,2-DICHLOROBENZENE	2005 ± 65	µg/mL	99.4	5	LB58923	95-50-1
BIS (2-CHLOROISOPROPYL) ETHER	2000 ± 45	µg/mL	96.7	6	LC19632	108-60-1
N-NITROSODI-N-PROPYLAMINE	2001 ± 36	µg/mL	100.0	7	2D5VJ-PB	621-64-7
HEXACHLOROETHANE	2000 ± 125	µg/mL	99.9	8	12719AO	67-72-1
NITROBENZENE	2000 ± 53	µg/mL	99.9	9	LB47070	98-95-3
ISOPHORONE	1999 ± 34	µg/mL	99.5	10	LC14006	78-59-1
BIS (2-CHLOROETHOXY) METHANE	2000 ± 33	µg/mL	98.7	11	LB46081	111-91-1
1,2,4-TRICHLOROBENZENE	2003 ± 91	µg/mL	99.9	12	447	120-82-1
HEXACHLOROBUTADIENE	1999 ± 97	µg/mL	97.2	13	MKCG6212	87-68-3
HEXACHLOROCYCLOPENTADIENE	2001 ± 111	µg/mL	96.0	14	LB95525	77-47-4
2-CHLORONAPHTHALENE	2000 ± 120	µg/mL	99.9	15	LC11403	91-58-7
DIMETHYL PHTHALATE	2006 ± 44	µg/mL	99.9	16	LB30494	131-11-3
2,6-DINITROTOLUENE	2000 ± 91	µg/mL	99.2	17	11231AN	606-20-2
2,4-DINITROTOLUENE	2000 ± 71	µg/mL	98.9	18	12316HF	121-14-2
DIETHYL PHTHALATE	1998 ± 51	µg/mL	99.9	19	207	84-66-2
4-CHLOROPHENYLPHENYL ETHER	2006 ± 52	µg/mL	99.3	20	JS00081	7005-72-3
N-NITROSODIPHENYLAMINE	2000 ± 72	µg/mL	95.5	21	LC07185	86-30-6
AZOBENZENE	2000 ± 48	µg/mL	98.2	22	BCBS6535V	103-33-3
4-BROMOPHENYLPHENYL ETHER	2006 ± 48	µg/mL	99.0	23	05916LS	101-55-3

ID #: 12503

Opened:

TCL Base-Neutrals Mix

Expires: 1/31/2023

Rec'd: 3/12/2020

Energy Laboratories Inc 1120 So. 27th Street
Billings MT 59107



SIGMA-ALDRICH

2931 Soldier Springs Rd. Laramie, Wyoming 82070 USA
800-325-5832
TechService@milliporesigma.com www.sigma-aldrich.com

RESTEK® CERTIFIED REFERENCE MATERIAL

110 Benner Circle
 Bellefonte, PA 16823-8812
 Tel: (800)356-1688
 Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31029 Lot No.: A0157111
 Description : 604 Phenols Calibration Mix
604 Calibration Std Phenols 2000µg/mL, Methanol, 1mL/ampul
 Container Size : 2 mL Pkg Amt: > 1 mL
 Expiration Date : January 31, 2028 Storage: 10°C or colder

ID #: 12512
 Opened: _____
 604 Phenols Calibration Mix
 Expires: 1/31/2028
 Rec'd: 3/17/2020
 Energy Laboratories Inc 1120 So. 27th Street
 Billings MT 59107

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight:volume)	Expanded Uncertainty (95% C.L., K=2)				
1	Phenol	2,004.0 µg/mL (Lot SHBF9719V)	+/-	11.9032	µg/mL	Gravimetric	
	CAS # 108-95-2		+/-	58.5341	µg/mL	Unstressed	
	Purity 99%		+/-	71.0092	µg/mL	Stressed	
2	2-Chlorophenol	2,000.0 µg/mL (Lot STBH7290)	+/-	11.8794	µg/mL	Gravimetric	
	CAS # 95-57-8		+/-	58.4173	µg/mL	Unstressed	
	Purity 99%		+/-	70.8674	µg/mL	Stressed	
3	2-Nitrophenol	2,000.0 µg/mL (Lot BCBH7602V)	+/-	11.8794	µg/mL	Gravimetric	
	CAS # 88-75-5		+/-	58.4173	µg/mL	Unstressed	
	Purity 99%		+/-	70.8674	µg/mL	Stressed	
4	2,4-Dimethylphenol	2,000.0 µg/mL (Lot 10165155)	+/-	11.8794	µg/mL	Gravimetric	
	CAS # 105-67-9		+/-	58.4173	µg/mL	Unstressed	
	Purity 99%		+/-	70.8674	µg/mL	Stressed	
5	2,4-Dichlorophenol	2,004.0 µg/mL (Lot BCBJ8113V)	+/-	11.9032	µg/mL	Gravimetric	
	CAS # 120-83-2		+/-	58.5341	µg/mL	Unstressed	
	Purity 99%		+/-	71.0092	µg/mL	Stressed	
6	4-Chloro-3-methylphenol	2,004.0 µg/mL (Lot STBC7309V)	+/-	11.9032	µg/mL	Gravimetric	
	CAS # 59-50-7		+/-	58.5341	µg/mL	Unstressed	
	Purity 99%		+/-	71.0092	µg/mL	Stressed	
7	2,4,6-Trichlorophenol	2,002.0 µg/mL (Lot STBH7520)	+/-	11.8913	µg/mL	Gravimetric	
	CAS # 88-06-2		+/-	58.4757	µg/mL	Unstressed	
	Purity 99%		+/-	70.9383	µg/mL	Stressed	

CERTIFICATE OF ANALYSIS

Catalog No: Z-014F
Description: Benzidine & 3,3'-Dichlorobenzidine
Lot: 220041353
Solvent: Methanol
Hazards: Refer to SDS for complete safety information

Date Certified: May 1, 2020
Expiration: May 1, 2024
Sample Size: 1 mL
Components: 2
Storage Condition: Ambient (>5 °C)



Signal Word: Danger

Certified Reference Material



Component	CAS #	Purity % (GC/MS)	Prepared Concentration ² (µg/mL)	Certified Analyte Concentration ¹ (µg/mL)
Benzidine **	92-87-5	99.9	2004	2002
3,3'-Dichlorobenzidine **	91-94-1	100.0	2001	2001

ID #: 12839

Opened: _____

Benzidine & 3,3'-Dichlorobenzidine

Expires: 5/1/2024

Rec'd: 7/7/2020

Energy Laboratories Inc 1120 So. 27th Street
Billings MT 59107

**Benzidine and 3,3'-Dichlorobenzidine are subject to oxidative degradation

**Benzidine and 3,3'-Dichlorobenzidine are subject to oxidative degradation

A product with a suffix (-1A, -2B, etc. or -01, -02, etc.) on its lot number has had its expiration date extended and is identical to the same lot number without the suffix.

² All weights are traceable through NIST, Test No. 684/289871-17

¹ Certified Analyte Concentration = Purity x Prepared Concentration.

The Uncertainty associated with the certified concentration reported on this certificate is $\pm 2.4\%$. This value is the combined expanded uncertainty and represents an estimated standard deviation equal to the positive square root of the total variation of the uncertainty of components. A normal distribution is assumed and a coverage factor of K=2 is chosen using approximately a 95% confidence level.

Labels and certificates follow U.S. Conventions in reporting numerical values: A comma (,) is used to separate units of one-thousand or greater. A period (.) is used as a decimal place marker.

The information on this certificate may not be reproduced without the express permission of the manufacturer. See reverse side for additional information

Certified By: _____

Larry Decker, Organic QC Manager

CERTIFICATE OF ANALYSIS

Catalog No: Z-014F
Description: Benzidine & 3,3'-Dichlorobenzidine
Lot: 220041353
Solvent: Methanol

Date Certified: May 1, 2020
Expiration: May 1, 2024
Sample Size: 1 mL
Components: 2

I-TEST

AccuStandard, Inc.
 Statistical Report for CLP (SOW 1997)
 1-May-2020

QR-CO-003 rev. 3/16

		Z-014F 220041353								Z-014F 220031213								NOTES:				
Peak	# Component	Run #1	Run #2	Run #3	Run #4	Mean	Std Dev	% RSD	Run #1	Run #2	Run #3	Run #4	Mean	Std Dev	% RSD	L029 test	CI 220041353	CI 220031213	# of Runs	10 % error check of Conc. means		
1	Benzidine (92-87-5)	90	83	79	78	83	5.45	6.60%	84	84	80	76	81	3.83	4.73%	0.45	23.7	Benzidine (92-87-5)	21.3	4	2000	2 %
2	3,3'-Dichlorobenzidine (91-94-1)	104	96	93	91	96	5.72	5.95%	98	99	94	89	95	4.27	4.51%	0.35	20.9	3,3'-Dichlorobenzidine (91-94-1)	15.8	4	2000	1 %

AccuStandard


CERTIFICATE OF ANALYSIS


Catalog No: Z-014F
Description: Benzidine & 3,3'-Dichlorobenzidine
Lot: 220041353
Solvent: Methanol

Date Certified: May 1, 2020
Expiration: May 1, 2024
Sample Size: 1 mL
Components: 2

Chromatogram

File :D:\MassHunter\GCMS\1\DATA\043020\14- 220041353.D
Operator : Organic QC Lab
Acquired : 30 Apr 2020 17:16 using AcqMethod CHICK_2019_S100.M
Instrument : GCMS 6
Sample Name: Z-014F (220041353)
Misc Info : Z-014F @2000ug/mL in Methanol
Vial Number: 138

 **AccuStandard®**
Leader in Analytical Reference Standards
Column: DB-5MS, 30m, 0.25 ID, 0.25 um
Oven Program: 80c 17c/min to 340c, 8min
GC Parameters: Cons. Split, 12psi constant flow
Split 100:1, 1uL inj.; GC/MS; INJ 270c

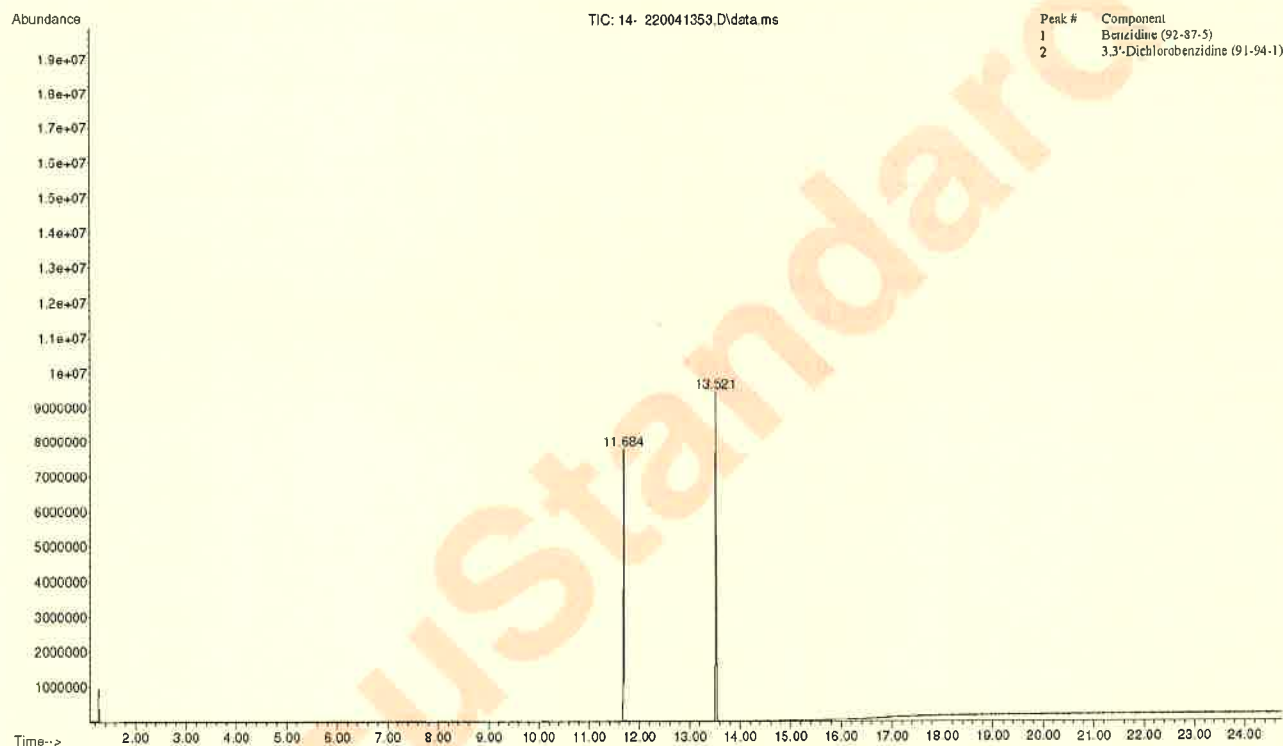

CERTIFICATE OF ANALYSIS

Catalog No: Z-014F
Description: Benzidine & 3,3'-Dichlorobenzidine
Lot: 220041353
Solvent: Methanol

Date Certified: May 1, 2020
Expiration: May 1, 2024
Sample Size: 1 mL
Components: 2

RAW DATA

Data Path : D:\MassHunter\GCMS\1\DATA\043020\
Data File : 14- 220041353.D
Acq On : 30 Apr 20 05:16 pm
Operator : Organic QC Lab
Sample : Z-014F (220041353)
Misc : Z-014F @2000ug/mL in Methanol
ALS Vial : 138 Sample Multiplier: 1

Integration Parameters: events.e
Integrator: ChemStation

Method : D:\MassHunter\GCMS\1\methods\CHICK_2019.M
Title :

Signal : TIC: 14- 220041353.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	11.684	2371	2386	2399	PV	7555441	90932217	86.94%	46.506%
2	13.521	2790	2799	2825	BB	9071921	104594086	100.00%	53.494%

Certificate of Analysis

Certified
Reference
Material

TCL PAH

MIX,1X1ML,2000UG/ML,BENZENE:DICHLOROMETHANE

Description

Product ID CRM48905
Lot LRAC3877
Expiration Date September 2022
Manufacturing Date September 2019
Storage Conditions Refrigerate
Solvent/Matrix methylene chloride: benzene (1:1)

Certified Values

Analyte	Certified Value ^{1,4}	Units	Raw Material Purity,%	Analytical Value ⁶	Elution order	Raw Material Lot	CAS
NAPHTHALENE	2000 ± 32	µg/mL	100.0	2022	01	01112017-5	91-20-
ACENAPHTHYLENE	2000 ± 66	µg/mL	99.8	2005	02	LC21494	208-96-
ACENAPHTHENE	2000 ± 63	µg/mL	99.9	2031	03	MKCC8329	83-32-
FLUORENE	2000 ± 90	µg/mL	99.4	2009	04	LC19126	86-73-
PHENANTHRENE	2000 ± 56	µg/mL	99.6	2043	05	MKCD3760	85-01-
ANTHRACENE	2000 ± 39	µg/mL	99.9	2005	06	LC14310	120-12-
FLUORANTHENE	2000 ± 69	µg/mL	98.5	2031	07	LB99099	206-44-
PYRENE	2000 ± 68	µg/mL	91.6	2078	08	LB70761	129-00-
BENZO (A) ANTHRACENE	2000 ± 63	µg/mL	99.9	2002	09	LC19271	56-55-
CHRYSENE	2000 ± 59	µg/mL	99.0	2026	10	21L74	218-01-
BENZO (B) FLUORANTHENE	2000 ± 62	µg/mL	99.5	1998	11	LB95773	205-99-
BENZO (K) FLUORANTHENE	2000 ± 62	µg/mL	99.9	2043	12	0000029501	207-08-
BENZO(A)PYRENE	2002 ± 64	µg/mL	99.6	2037	13	LB73826	50-32-
DIBENZ (A,H) ANTHRACENE	2000 ± 64	µg/mL	99.0	2050	14	0012014	53-70-
BENZO (G,I,I) PERYLENE	2000 ± 67	µg/mL	98.5	2059	15	LC19498	191-24-
INDENO (1,2,3-CD) PYRENE	2000 ± 64	µg/mL	99.5	1995	16	ER082107-02	193-39-

ID #: 12846

Opened: _____

TCL PAH

Expires: 9/30/2022

Rec'd: 7/13/2020

Eneray Laboratories Inc 1120 So. 27th Street
Billings MT 59107




SIGMA-ALDRICH
2931 Soldier Springs Rd. Laramie, Wyoming 82070 USA
307-742-5452
rtctechgroup@sial.com www.sigma-aldrich.com

Description

Lot LRAC3877
 Expiration Date September 2022
 Manufacturing Date September 2019
 Storage Conditions Refrigerate
 Solvent/Matrix methylene chloride: benzene (1:1)

Informational Values



Additional Information:

Analytical Method Parameters:
 Column: Supelco LC-PAH, 250 mm x 4.6mm, 5µm particle size
 Mobile Phase A: Water
 Mobile Phase B: Acetonitrile
 Detector: UV/DAD/VWD, Wavelength: 254 nm
 Flow Rate: 1.7 mL/min
 Column Temperature: 30 °C
 Injection Volume: 2 µL

Gradient

TIME (min)	A%	B%
0	40	60
5	40	60
30	0	100
45	0	100
50	40	60

Certificate of Analysis

Certified
Reference
Material

TCL PAH

MIX,1X1ML,2000UG/ML,BENZENE:DICHLOROMETHANE

Description

Product ID CRM48905
Lot LRAC3877
Expiration Date September 2022
Manufacturing Date September 2019
Storage Conditions Refrigerate
Solvent/Matrix methylene chloride: benzene (1:1)

1 Metrological traceability: Traceable to the SI and higher order standards from NIST through an unbroken chain of comparisons. The balance used to weigh raw materials is accurate to +/-0.0001 g and calibrated regularly using mass standards traceable to NIST. All dilutions were performed gravimetrically. Additionally, individual analytes are traceable to NIST SRMs where available and specified above.
4 Ucrm - Uncertainty values in this document are expressed as Expanded Uncertainty (Ucrm) corresponding to the 95% confidence interval. Ucrm is derived from the combined standard uncertainty multiplied by the coverage factor k, which is obtained from a t-distribution and degrees of freedom. The components of combined standard uncertainty include the uncertainties due to characterization, homogeneity, long term stability, and short term stability (transport). The components due to stability are generally considered to be negligible unless otherwise indicated by stability studies. The mathematical representation of the Ucrm calculation is as follows:

$$u_{CRM} = \sqrt{u_{char}^2 + u_{homogeneity}^2 + u_{stability}^2}$$

k: Coverage factor derived from a t-distribution table, based on the degrees of freedom of the data set. Assume 2.0 for a **Confidence interval = 95%**

6 Analytical Value- For QC verification of the certified value only- not to be used in calculations. Represents the analytical data obtained by comparison to a standard as analyzed by the method described in the CoA or another acceptable method. The result may differ from the certified value and UCRM based on method uncertainty as well as the uncertainty associated with the standard used for comparison.

Traceability: The standard was manufactured under an ISO/IEC 17025:2017 certified quality system. The balance used to weigh raw materials is accurate to +/- 0.0001g and calibrated regularly using mass standards traceable to NIST. All dilutions were performed gravimetrically. Additionally, individual analytes are traceable to NIST SRMs where available and specified above.

Homogeneity: Homogeneity was assessed in accordance with ISO 17034:2016. Completed units were sampled using a random stratified sampling protocol. The results of chemical analysis were then compared using a one-way analysis of variance approach as described by TNI EL-V3-2009 Appendix A.2. See Instructions for minimum sub-sample size.


Expiration is at end of month given on certificate and label.

THIS PRODUCT WAS DESIGNED, PRODUCED AND VERIFIED FOR ACCURACY AND STABILITY IN ACCORDANCE WITH **ISO/IEC 17025:2017 (ANAB Cert AT-1467)** and **ISO 17034:2016 (ANAB Cert AR-1470)**.

MSDS reports for components comprising greater than 1.0% of the solution or 0.1% for components known to be carcinogens are available upon request.



Andy Ommen - QC Manager



Mark Pooler - QA Supervisor

Certification Date October 17, 2019
Version 0-10172019



SIGMA-ALDRICH

2931 Soldier Springs Rd. Laramie, Wyoming 82070 USA
307-742-5452
rtctechgroup@sial.com www.sigma-aldrich.com



CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31086 **Lot No.:** A0166081

Description : B/N Surrogate Mix (4/89 SOW)
Base Neutral Surrogate 5000µg/mL, Methylene Chloride, 5mL/ampul

Container Size : 5 mL **Pkg Amt:** > 5 mL

Expiration Date : October 31, 2026 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

ID #: 13328
Opened: _____
B/N Surrogate Mix (4/89 SOW)
Expires: 10/31/2026
Rec'd: 12/14/2020
Enerav Laboratories Inc 1120 So. 27th Street
Billings MT 59107

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)			
1	Nitrobenzene-d5 CAS # 4165-60-0 Purity 99% (Lot PR-29940B)	5,017.7 µg/mL	+/-	29.1731	µg/mL	Gravimetric
			+/-	225.9987	µg/mL	Unstressed
			+/-	250.7735	µg/mL	Stressed
2	2-Fluorobiphenyl CAS # 321-60-8 Purity 99% (Lot 00019169)	5,049.7 µg/mL	+/-	29.3592	µg/mL	Gravimetric
			+/-	227.4400	µg/mL	Unstressed
			+/-	252.3728	µg/mL	Stressed
3	p-Terphenyl-d14 CAS # 1718-51-0 Purity 99% (Lot PR-27278)	5,029.9 µg/mL	+/-	29.2444	µg/mL	Gravimetric
			+/-	226.5505	µg/mL	Unstressed
			+/-	251.3857	µg/mL	Stressed

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

Tech Tips:

Due to the limited solubility of p-terphenyl-d14 in methanol, we do not recommend that this mixture be diluted in methanol.

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

40°C (hold 2 min.) to 330°C
@ 10°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

330°C

Det. Type:

FID

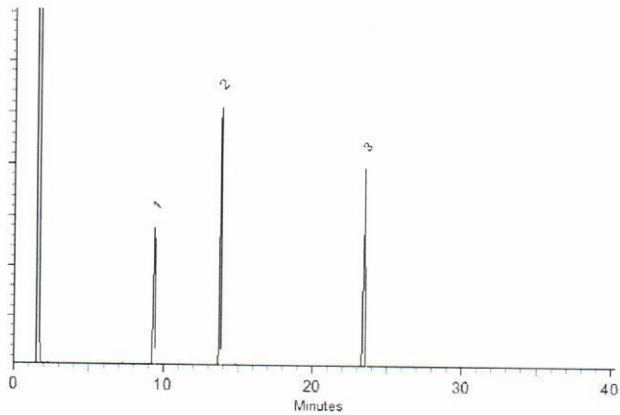

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Dalton Stover - Operations Technician I

Date Mixed: 04-Nov-2020

Balance: 1128353505

Justine Albertson - Operations Tech-ARM QC

Date Passed: 06-Nov-2020

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value (includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at www.restek.com/Contact-Us for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at www.restek.com/Contact-Us.
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.

660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599
1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729
info@chemservice.com • www.chemservice.com

ID #: 13372

Opened:

Mixture #8-Internal Standards

Expires: 5/31/2022

Rec'd: 12/29/2020

Energy Laboratories Inc 1120 So. 27th Street
Billings MT 59107

CERTIFICATE OF ANALYSIS

Mixture #8-Internal Standards

CONCENTRATION 4000ug/ml in Methylene chloride
CATALOG NUMBER M-PPHC8X12-1ML
LOT NUMBER 10051700
DATE CERTIFIED 05/13/20
EXPIRATION DATE 05/31/22
STORAGE Store at room temperature (20 - 25 °C).
HANDLING See Safety Data Sheet
INTENDED USE For laboratory use only.
ISO 17034:2016 CERTIFIED [X]

ID	Analyte	CAS	Weight Analyte (mg)	Lot	Purity	Certified Concentration (ug/mL)
N-11000	Acenaphthene-d10	15067-26-2	1005.50	00027326	99.50	4001.9
N-11467	Chrysene-d12	1719-03-5	1012.20	00027327	98.80	4000.2
N-10217	1,4-Dichlorobenzene-d4	3855-82-1	1004.10	00027328	99.50	3996.3
N-12645	Naphthalene-d8	1146-65-2	1006.50	00025577	99.50	4005.9
N-12851	Perylene-d12	1520-96-3	1009.50	00027330	99.50	4017.8
N-12856	Phenanthrene-d10	1517-22-2	1021.10	00027331	99.00	4043.6

Analytical Test

CONCENTRATION (GC/FID)

Value

VERIFIED

Instructions for Use:

Shake mixture prior to use. If particles are present, sonicate for homogeneity. If sample is diluted to lower concentrations, Class A volumetric glassware must be used.

Minimum Sample Size- 0.2 uL for Direct Injection.

Chem Service Inc. guarantees the expanded uncertainty of the above analytes to be +/- 2.0% of the certified concentrations based on gravimetric preparation. The test results published in this report were obtained using equipment capable of producing results that are traceable to NIST and through NIST to the International System of Units (SI). The reported expanded uncertainty of measurement is stated as the combined standard uncertainty of measurement multiplied by the coverage factor k (k=2) such that the coverage probability corresponds to approximately 95%. For certified reference materials, homogeneity and thermal stability testing are available upon request.

Certified By:

Mary Beth O'Donnell

Mary Beth O'Donnell
CSM/TC

Chem Service is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015



COA Form
Revision 3 (3/2015)


660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599
 1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729
info@chemservice.com • www.chemservice.com

Gas

Data file: C:\CHEM3\
 Sample name: M-PPCH8X
 Instrument: GC 2
 Injection date: 5/13/2020 8:56:25 AM
 Acq. method: M-PPHC8X12.M
 Column name: HP-5

CERTIFICATE OF ANALYSIS

Sample type: Sample
 Location: Vial 3
 Injection volume: 1.0uL



Signal: FID1 A, Front Signal

RT [min]	Type	Width [min]	Area	Height	Area%
5.427	BB	0.0181	1240.1130	1041.0874	8.36
6.593	BB	0.0189	2274.8877	1876.2654	15.33
8.272	BB	0.0196	2371.0022	1888.8049	15.98
9.696	BV	0.0197	2694.9399	2106.0442	18.16
12.654	BB	0.0330	2999.0918	1397.3110	20.21
16.001	BB	0.0562	3260.5679	751.0330	21.97
		Sum	14840.6025		

Chem Service is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015





CERTIFIED REFERENCE MATERIAL

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: (800)356-1688
Fax: (814)353-1309

www.restek.com

Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 31062 **Lot No.:** A0167670

Description : B/N Surrogate Mix (4/89 SOW)
Base Neutral Surrogate 4/89(SOW) 5000µg/mL, Methylene Chloride, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : November 30, 2026 **Storage:** 10°C or colder

Handling: Sonicate prior to use. **Ship:** Ambient

CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)			
1	Nitrobenzene-d5 CAS # 4165-60-0 Purity 99% (Lot PR-29940B)	5,014.0 µg/mL	+/-	29.3583	µg/mL	Gravimetric
			+/-	225.8621	µg/mL	Unstressed
			+/-	250.6163	µg/mL	Stressed
2	2-Fluorobiphenyl CAS # 321-60-8 Purity 99% (Lot 00019169)	5,019.6 µg/mL	+/-	29.3911	µg/mL	Gravimetric
			+/-	226.1143	µg/mL	Unstressed
			+/-	250.8962	µg/mL	Stressed
3	p-Terphenyl-d14 CAS # 1718-51-0 Purity 99% (Lot PR-27278)	5,020.6 µg/mL	+/-	29.3967	µg/mL	Gravimetric
			+/-	226.1576	µg/mL	Unstressed
			+/-	250.9442	µg/mL	Stressed

Solvent: Methylene chloride
CAS # 75-09-2
Purity 99%

ID #: 13666

Opened: _____

B/N Surrogate Mix (4/89 SOW)

Expires: 11/30/2026

Rec'd: 3/19/2021

Energry Laboratories Inc 1120 So. 27th Street
Billings MT 59107

Tech Tips:

Due to the limited solubility of p-terphenyl-d14 in methanol, we do not recommend that this mixture be diluted in methanol.

Column:

30m x 0.25mm x 0.25µm
Rtx-5 (cat.#10223)

Carrier Gas:

hydrogen-constant pressure 10 psi.

Temp. Program:

75°C (hold 1 min.) to 330°C
@ 20°C/min. (hold 10 min.)

Inj. Temp:


250°C

Det. Temp:

330°C

Det. Type:

FID



This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Katelyn McGinni - Operations Tech I

Date Mixed: 30-Dec-2020 Balance: 1128353505


Alexis Shelow - Operations Tech I

Date Passed: 06-Jan-2021

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value (includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at www.restek.com/Contact-Us for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at www.restek.com/Contact-Us.
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.


Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.

Certificate of Analysis - Certified Reference Material

EPA TCL Hazardous Substances Mix (12 cmpds)

Product no.: 47990-U
Lot no.: LRAC9004
Expiry Date: February 2024
Manufacturing Date: February 2021
Storage: Refrigerate
Solvent/Matrix: Dichloromethane
Certificate version: LRAC9004.01 (Note: Certificates may be updated due to the availability of new data. Check our website at: www.sigma-aldrich.com for the most current version.)



Certified Values:

Analyte	Certified Value	Units	Raw Material Purity, %	Raw Material Elution order	Raw Material Lot
ANILINE CAS# 62-53-3	2022 ± 25	µg/mL	99.9	01	LA41596
BENZYL ALCOHOL CAS# 100-51-6	2022 ± 15	µg/mL	99.7	02	LB99705
2-METHYLPHENOL CAS# 95-48-7	2022 ± 14	µg/mL	99.9	03	LB91878
4-METHYLPHENOL CAS# 106-44-5	2022 ± 17	µg/mL	99.9	04	LB32518
BENZOIC ACID CAS# 65-85-0	2021 ± 27	µg/mL	98.8	05	442-137B
4-CHLOROANILINE CAS# 106-47-8	2022 ± 32	µg/mL	100.0	06	MKBZ6909V
2,4,5-TRICHLOROPHENOL CAS# 95-95-4	2022 ± 18	µg/mL	99.9	07	JS00008
2-METHYLNAPHTHALENE CAS# 91-57-6	2021 ± 11	µg/mL	98.2	08	LB97828
2-NITROANILINE CAS# 88-74-4	2022 ± 12	µg/mL	99.9	09	07411KN
3-NITROANILINE CAS# 99-09-2	2022 ± 15	µg/mL	99.9	10	LC09264
DIBENZOFURAN CAS# 132-64-9	2021 ± 10	µg/mL	98.8	11	LB78814
4-NITROANILINE CAS# 100-01-6	2022 ± 23	µg/mL	99.9	12	15609AA

ID #: 13691

Opened:

EPA TCL Hazardous Substances Mix (12 cmp)


Expires: 2/28/2024

Rec'd: 3/26/2021

Energv Laboratories Inc 1120 So. 27th Street
Billings MT 59107



Informational Values:

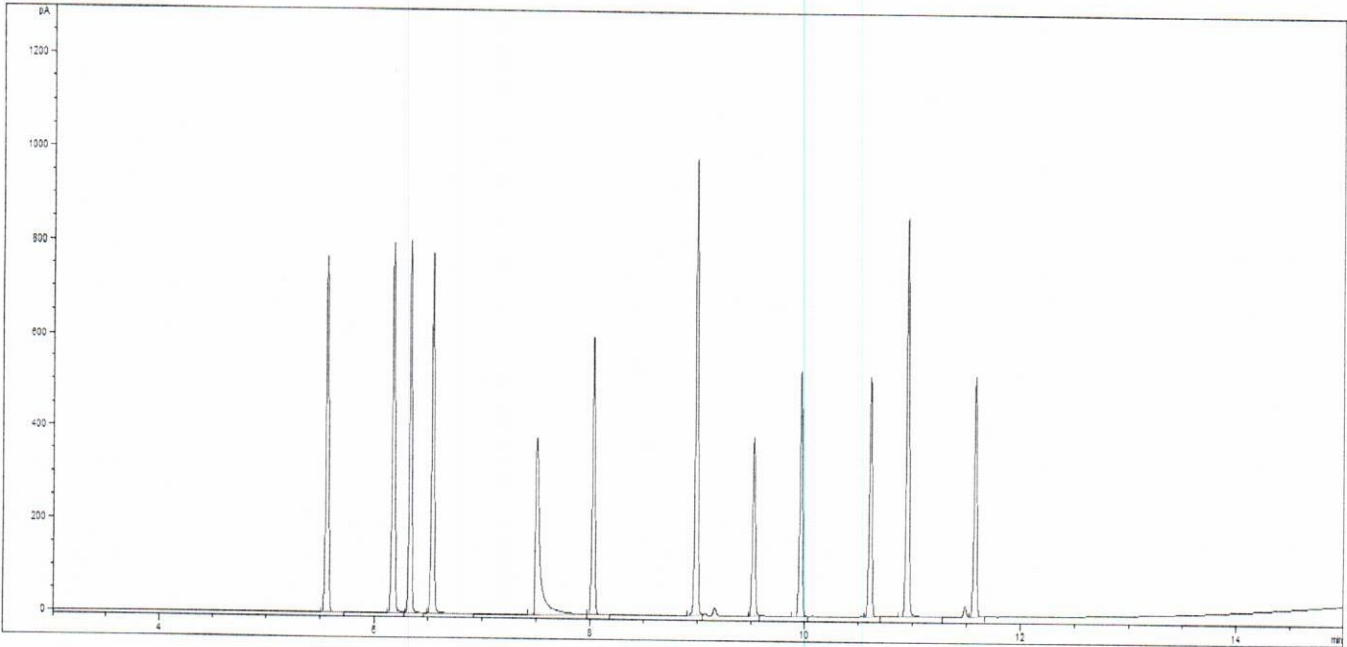

Additional Information:

Analytical Method Parameters:
Column: SPB-5, 30 m x 0.53 mm I.D., 1.5 µm film thickness (Column #214)
Carrier Gas: H₂, Flow: 4.5 mL/min
Inlet Temperature: 240 °C, Injection Volume: 1 µL
Injection Mode: Split, Split Ratio: 25:1
Temperature Program: 80 °C (Hold 2 min) @ 15 °C/min to 280 °C (Hold 2 min)
Detector: FID
Detector Temperature: 310 °C

Metrological traceability:

Traceable to the SI and higher order standards from NIST through an unbroken chain of comparisons. The balance used to weigh raw materials is accurate to +/-0.0001 g and calibrated regularly using mass standards traceable to NIST. All dilutions were performed gravimetrically. Additionally, individual analytes are traceable to NIST SRMs where available and specified above.

Measurement method:

Where applicable, the assigned value is based on a purity determination by mass balance and gravimetrically prepared value.

Intended use:

Intended for R&D and Analytical Use only. Not for drug, household or other uses.

Minimum sample size:

1 µL

Packaging:

1 ML IN AMBER AMPULE

Instructions for handling and correct use:

Use on the as is basis. The internal pressure of the container may be slightly different from the atmospheric pressure at the user's location. Open slowly and carefully to avoid dispersion of the material.

Health and safety information:

All chemical reference materials should be considered potentially hazardous and should be used only by qualified laboratory personnel. Please refer to the Safety Data Sheet for detailed information about the nature of any hazard and appropriate precautions to be taken.

Accreditation:

Sigma-Aldrich RTC is accredited by the US accreditation authority ANAB as a registered reference material producer AR-1470 in accordance with ISO 17034.

Certificate issue date:

26-Feb-2021



Andy Ommen - QC Manager

Mark Pooler - QA Supervisor

Details on metrological traceability:

This standard has been gravimetrically prepared using balances that have been fully qualified and calibrated to ISO 17025 requirements. All calibrations utilize NIST traceable weights which are calibrated externally by a qualified ISO 17025 accredited calibration laboratory to NIST standards. Qualification of each balance includes the assignment of a minimum weighing by a qualified and ISO 17025 accredited calibration vendor taking into consideration the balance and installed environmental conditions to ensure compliance with USP tolerances of NMT 0.10% relative error. Fill volume to predetermined specifications is gravimetrically verified throughout the dispensing process using qualified and calibrated balances. Further traceability to a corresponding Primary Standard may be achieved through a direct comparison assay. Where a Primary Standard is available, the assay value will be included in the specified section of the COA.

Details on metrological traceability:

Ucrm - Uncertainty values in this document are expressed as Expanded Uncertainty (Ucrm) corresponding to the 95% confidence interval. Ucrm is derived from the combined standard uncertainty multiplied by the coverage factor k, which is obtained from a t-distribution and degrees of freedom. The components of combined standard uncertainty include the uncertainties due to characterization, homogeneity, long term stability, and short term stability (transport). The components due to stability are generally considered to be negligible unless otherwise indicated by stability studies. The mathematical

$$u_{CRM} = \sqrt{u_{char}^2 + u_{homogeneity}^2 + u_{stability}^2}$$

Homogeneity assessment:

Homogeneity was assessed in accordance with ISO Guide 35. Completed units were sampled using a random stratified sampling protocol. The results of chemical analysis were then compared by Single Factor Analysis of Variance (ANOVA). The uncertainty due to homogeneity was derived from the ANOVA. Heterogeneity was not detected under the conditions of the ANOVA.

Stability assessment:

Significance of the stability assessment will be demonstrated if the analytical result of the study and the range of values represented by the Expanded Uncertainty do not overlap the result of the original assay and the range of its values represented by the Expanded Uncertainty. The method employed will usually be the same method used to characterize the assay value in the initial

Certificate of analysis revision history:

Certificate version	Date	Reason for version
LRAC9004.01	26-Feb-2021	Original Release Date

Disclaimer: The purchaser is required to determine the suitability of this product for any particular application. Sigma-Aldrich RTC makes no warranty of any kind, express or implied, other than its products meet all quality control standards set by Sigma-Aldrich RTC. We do not guarantee that the product can be used for any particular application.

The vibrant M, Supelco, TraceCERT and Sigma-Aldrich are trademarks of Merck KGaA, Darmstadt, Germany or its affiliates. All other trademarks are the property of their respective owners. Detailed information on trademarks is available via publicly accessible resources. © 2018 Merck KGaA, Darmstadt, Germany and/or its affiliates. All Rights Reserved.

The life science business of Merck KGaA, Darmstadt, Germany operates as MilliporeSigma in the US and Canada.



Certificate of Analysis

Product Name: Benzidines Standard
Product Number: US-290-1
Lot Number: 0006592783

Lot Issue Date: 03-Mar-2021
Expiration Date: 30-Apr-2023

Description:

This analytical reference material (RM) was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed below.

Analyte	CAS#	Analyte Lot	Concentration ± Uncertainty
benzidine	000092-87-5	RM10200	2004 ± 10 µg/mL
3,3'-dichlorobenzidine	000091-94-1	RM12559	2001 ± 10 µg/mL

Matrix: methylene chloride (dichloromethane)

Storage Conditions: Store at Room Temperature (15° to 30°C).

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCCL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This RM was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Intended Use:

This RM is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Hazards:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this RM.


Expiration of Certification:

The certification of this RM is valid until the expiration date specified above, provided the RM is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the RM is damaged, contaminated, or otherwise modified.

Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:



Monica Bourgeois
 QMS Representative



ISO 17034 Cert
 No. AR-1936

RM was produced in accordance with the LRQA registered ISO 9001:2015 Quality Management System. Cert # 10303760

Page: 1 of 1

www.agilent.com/quality/
 CSD-QA-015.1



ISO 17025 Cert
 No. AT-1937




Run 19, "P92180 L020221 [1000µg/mL in MeCl2]"

Run Length: 40.00 min, 23999 points at 10 points/second.
Created: Sat, Feb 6, 2021 at 4:44:57 AM
Sampled: Sequence 020521-GC4M2, Method GC4-M2
Analyzed using Method GC4-M2

Comments

GC4-M2 Analysis by Melissa Stonier
Column ID: SFR-5 L#60062-01A 30 meter x 0.53mm x 1.5µm Film Thickness
Flow rates: Total Flow = 300 mL/min, Helium (Carrier) = 6.5 mL, Helium (make-up) = 25 mL
Hydrogen (Detector) = 30 mL, Air (Detector) = 360 mL, Oven Temp 1 = 50°C (1 min)
Rate = 10°C/min, Oven Temp 2 = 300°C (14 min), Total Run Time = 40 Minutes, Injector Temp = 250°C,
FID Temp = 300°C, FID Signal = eDAQ Channel 1
Gas Chromatograph = HP 5990, Auto Sampler = HP 7673, Standard Injection = 0.5 µL, Range = 3



Peak No.	Name	FID RT (min)
1	N-nitrosodimethylamine	4.30
2	Pyrene	8.05
3	Di(2-Chloroethyl)ether	8.25
4	2-Chlorophenol	8.40
5	1,3-Dichlorobenzene	8.71
6	1,4-Dichlorobenzene	8.80
7	1,3-Dichlorobenzene	9.19
8	o-Cresol (2-methylphenol)	9.27
9	Di(2-Chloroethyl)ether	9.38
10	p-Cresol (4-methylphenol) [N-nitrosodimethylamine]	9.50
11	Hexachlorobenzene	9.70
12	Nitrobenzene	9.85
13	Isobutylene	10.02
14	2-Nitrophenol	10.53
15	2,4-Dimethylphenol	10.74
16	Di(2-Chloroethyl)ether	10.81
17	2,4-Dichlorophenol	10.87
18	1,2,4-Trichlorobenzene	11.31
19	Naphthalene	11.43
20	4-Chlorophenol	11.57
21	Hexachloro-1,3-butadiene	11.70
22	4-Chloro-3-methylphenol	11.86
23	2-Methylnaphthalene	12.77
24	Hexachlorocyclopentadiene	13.14
25	2,4,6-Trichlorophenol	13.65
26	2,4,5-Trichlorophenol	13.83
27	2-Chloronaphthalene	13.91
28	2-Nitroaniline	14.26
29	Dimethyl phthalate	14.56
30	Acenaphthylene	15.05
31	2,6-Dimethylamine	15.25
32	3-Nitroaniline	15.54
33	Acenaphthene	15.69
34	2,4-Dichlorophenol	15.77
35	Dibenz(a,h)anthracene	15.89
36	2,4-Dinitrobenzene	16.06
37	Diethyl pthalate/fluorene	16.14
38	4-Chlorophenyl phenyl ether	16.72
39	4-Nitroaniline	16.87
40	4,6-Dinitro-2-methylphenol	17.00
41	Azobenzene	17.09
42	4-Bromophenyl phenyl ether	17.23
43	Hexachlorobenzene	18.00
44	Pentachlorophenol	18.96
45	Phenanthrene	18.76
46	Anthracene	19.13
47	Carbazole	19.24
48	Dimethyl phthalate	19.61
49	Fluoranthene	20.35
50	Pyrene	21.96
51	Benzyl butyl phthalate	22.69
52	Benz(a)anthracene	24.11
53	Chrysene	25.34
54	Di(2-Ethylhexyl)phthalate	25.45
55	Di-n-octyl phthalate	25.52
56	Benz(b)fluoranthene	26.98
57	Benz(a)fluoranthene	28.16
58	Benz(a)pyrene	29.10
59	Indeno(1,2,3-cd)perylene/Benz(a,h)anthracene	33.79
60	Benz(g,h)perylene	35.02

CERTIFICATE OF ANALYSIS

Catalog No: S-14500-R2
Description: Custom Semi-Volatile Standard
Lot: 220021255-02
Solvent: Dichloromethane
Hazards: Refer to SDS for complete safety information

Date Certified: Aug 31, 2021
Expiration: Oct 1, 2022
Sample Size: 1 mL
Components: 10
Storage Condition: Freeze (<-10 °C)/Sonicate



Certified Reference Material



Component	CAS #	Purity % (GC/MS)	Prepared Concentration ² (µg/mL)	Certified Analyte Concentration ¹ (µg/mL)
Pyridine				
4-Chlorophenol	110-86-1	98.7	2026	2000
1-Methylnaphthalene	106-48-9	100.0	2019	2019
N-Nitrosodiphenylamine	90-12-0	98.5	2003	1973
4-Chloro-2-methylphenol	86-30-6	100.0	2022	2022
Benzoic acid	1570-64-5	97.0	2069*	2007
Aniline	65-85-0	99.5	2010	2000
Benzyl alcohol	62-53-3	98.0	2002	1962
Triallate	100-51-6	99.9	2011	2009
o-Terphenyl	2303-17-5	99.9	2013	2011
	84-15-1	99.9	2019	2017

ID #: 14279
Opened: _____
Custom Semi-Volatile Standard
Expires: 10/1/2022
Rec'd: 9/16/2021
Enerav Laboratories Inc 1120 So. 27th Street
Billings MT 59107

This Certified Reference Material was verified in accordance with ISO/IEC 17025

* Weight compensated to 100% purity.

A product with a suffix (-1A, -2B, etc. or -01, -02, etc.) on its lot number has had its expiration date extended and is identical to the same lot number without the suffix.

² All weights are traceable through NIST, Test No. 684/289871-17

¹ Certified Analyte Concentration = Purity x Prepared Concentration.


The Uncertainty associated with the certified concentration reported on this certificate is ±2.4%. This value is the combined expanded uncertainty and represents an estimated standard deviation equal to the positive square root of the total variation of the uncertainty of components. A normal distribution is assumed and a coverage factor of K=2 is chosen using approximately a 95% confidence level.

Labels and certificates follow U.S. Conventions in reporting numerical values: A comma (,) is used to separate units of one-thousand or greater. A period (.) is used as a decimal place marker.

The information on this certificate may not be reproduced without the express permission of the manufacturer. See reverse side for additional information

Hazard Information: Please refer to the SDS for information regarding the hazards associated with using this material.

This product was prepared according to in-house procedures and is guaranteed to be homogeneous.

Certified By: 
Larry Decker, Organic QC Manager