

# Energy Laboratories Inc

# ANALYTICAL RUN Summary

28-Feb-22

Run ID VOA5975C.I\_220104A

Run Start Date: 1/4/2022  
 Analyst: Melissa Chavez  
 Ical:  
 Column ID:  
 Comments:

| Instrument ID | Description |
|---------------|-------------|
| Bal #22       | Balance     |

| Std ID    | Std Name                                  | Std Amount | Std Units | Samp Amount | Samp Units | SampType    | Expiration Date |
|-----------|-------------------------------------------|------------|-----------|-------------|------------|-------------|-----------------|
| VOCF3473  | Calibration Surrogates                    |            | ul        | 42          | ml         | CAL         | 3/14/2022       |
| VOCF3517  | Internal Standard / Surrogates (INT/SURR) | 8.4        | ul        | 42          | ml         | MBLK, ICV ( | 12/31/2022      |
| VOCF3529B | 2nd Source MtBE                           | 1.05       | ul        | 42          | ml         | ICV         | 1/29/2022       |
| VOCF3546A | Liquids                                   |            | ul        | 42          | ml         | CAL         | 1/13/2022       |
| VOCF3549  | 2nd Source Ketones                        | 1.05       | ul        | 42          | ml         | ICV         | 1/15/2022       |
| VOCF3550  | Ketones                                   |            | ul        | 42          | ml         | CAL         | 1/16/2022       |
| VOCF3558B | 2nd Source Liquids                        | 1.05       | ul        | 42          | ml         | ICV         | 2/27/2022       |
| VOCF3559A | MtBE                                      |            | ul        | 42          | ml         | CAL         | 1/27/2022       |
| VOCF3562A | Gases                                     |            | ul        | 42          | ml         | CAL         | 1/10/2022       |
| VOCF3563  | Internals                                 | 8.4        | ul        | 42          | ml         | CAL         | 7/3/2022        |
| VOCF3566A | 2nd Source Gases                          | 1.05       | ul        | 42          | ml         | ICV         | 1/11/2022       |

| Seq No             | Lab ID       | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |       |      |   |
|--------------------|--------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|-------|------|---|
| 14970784           | 04JAN08_D_TU | VOC-8260-BFB | TUNE       | DA5975C\VG010: | 1/4/2022 2:38:00 | 1     | R372940  |           | 0      | 0      |        |      |     |       |      |   |
| Analyte            | T            | Units        | RAW        | Final          | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH  | %RPD | Q |
| 173, % of mass 174 | A            | %            | 0          | 0              |                  | 100   | 0        | 0         | 0      | 0      | 0      | 0%   | 0   | 1.99  | 0%   |   |
| 174, % of mass 95  | A            | %            | 95.2       | 95.2           |                  | 100   | 0        | 0         | 0      | 0      | 0      | 95%  | 50  | 99.99 | 0%   |   |
| 175, % of mass 174 | A            | %            | 6.6        | 6.6            |                  | 100   | 0        | 0         | 0      | 0      | 0      | 7%   | 5   | 9     | 0%   |   |
| 176, % of mass 174 | A            | %            | 95.7       | 95.7           |                  | 100   | 0        | 0         | 0      | 0      | 0      | 96%  | 95  | 101   | 0%   |   |
| 177, % of mass 176 | A            | %            | 6.7        | 6.7            |                  | 100   | 0        | 0         | 0      | 0      | 0      | 7%   | 5   | 9     | 0%   |   |
| 50, % of mass 95   | A            | %            | 21.2       | 21.2           |                  | 100   | 0        | 0         | 0      | 0      | 0      | 21%  | 15  | 40    | 0%   |   |
| 75, % of mass 95   | A            | %            | 51         | 51             |                  | 100   | 0        | 0         | 0      | 0      | 0      | 51%  | 30  | 60    | 0%   |   |
| 95, Base Peak      | A            | %            | 100        | 100            |                  | 100   | 0        | 0         | 0      | 0      | 0      | 100% | 0   | 100   | 0%   |   |
| 96, % of mass 95   | A            | %            | 5.4        | 5.4            |                  | 100   | 0        | 0         | 0      | 0      | 0      | 5%   | 5   | 9     | 0%   |   |

| Seq No                    | Lab ID      | Test Code    | Sample Typ | File ID       | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|---------------------------|-------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970898                  | MBLK010422_ | VOC-8260-W-Q | MBLK       | DA5975CVVG010 | 1/4/2022 3:05:37 | 1     | R372940  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                   | T           | Units        | RAW        | Final         | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.101  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 1,1,1-Trichloroethane     | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.131  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 1,1,2,2-Tetrachloroethane | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0872 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 1,1,2-Trichloroethane     | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.108  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 1,1-Dichloroethane        | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.135  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 1,1-Dichloroethene        | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.141  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 1,1-Dichloropropene       | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.083  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 1,2,3-Trichloropropane    | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.235  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 1,2-Dibromoethane         | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0916 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 1,2-Dichlorobenzene       | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0746 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 1,2-Dichloroethane        | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.116  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 1,2-Dichloropropane       | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0847 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 1,3-Dichlorobenzene       | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0803 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 1,3-Dichloropropane       | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0791 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 1,4-Dichlorobenzene       | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0858 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 2,2-Dichloropropane       | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.186  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 2-Chlorotoluene           | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0876 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 4-Chlorotoluene           | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0728 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Benzene                   | A           | ug/L         | 0.12327    | 0             |                  | 0     | 0        | 0         | 0.0914 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Bromobenzene              | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0831 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Bromochloromethane        | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.141  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Bromodichloromethane      | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.12   | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Bromoform                 | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.119  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Bromomethane              | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.253  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Carbon tetrachloride      | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.143  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Chlorobenzene             | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0914 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Chlorodibromomethane      | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0841 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Chloroethane              | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.169  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Chloroform                | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0789 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Chloromethane             | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.162  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| cis-1,2-Dichloroethene    | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.108  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| cis-1,3-Dichloropropene   | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.073  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Dibromomethane            | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.147  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Dichlorodifluoromethane   | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.175  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Ethylbenzene              | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0836 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |

| Seq No                         | Lab ID      | Test Code    | Sample Typ | File ID       | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|--------------------------------|-------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970898                       | MBLK010422_ | VOC-8260-W-Q | MBLK       | DA5975C\VG010 | 1/4/2022 3:05:37 | 1     | R372940  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                        | T           | Units        | RAW        | Final         | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| m+p-Xylenes                    | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.15   | 0.5    | 1000   | 0%   | 0   | 0    | 0%   |   |
| Methyl ethyl ketone            | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 1.77   | 10     | 5000   | 0%   | 0   | 0    | 0%   |   |
| Methyl tert-butyl ether (MTBE) | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.101  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Methylene chloride             | A           | ug/L         | 1.44235    | 0             |                  | 0     | 0        | 0         | 0.338  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| o-Xylene                       | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0604 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Styrene                        | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.067  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Tetrachloroethene              | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0671 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Toluene                        | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0679 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| trans-1,2-Dichloroethene       | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.125  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| trans-1,3-Dichloropropene      | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0846 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Trichloroethene                | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0993 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Trichlorofluoromethane         | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.134  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Vinyl chloride                 | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.153  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 1,4-Dichlorobenzene-d4         | I           | ug/L         | 250        | 10            |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 0   | 0    | 0%   |   |
| Chlorobenzene-d5               | I           | ug/L         | 250        | 10            |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 0   | 0    | 0%   |   |
| Fluorobenzene                  | I           | ug/L         | 250        | 10            |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 0   | 0    | 0%   |   |
| Xylenes, Total                 | M           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0604 | 0.5    | 1500   | 0%   | 0   | 0    | 0%   |   |
| 1,2-Dichloroethane-d4          | S           | ug/L         | 279.39635  | 11.175854     |                  | 10    | 0        | 0         | 0.229  | 0.5    | 500    | 112% | 70  | 130  | 0%   |   |
| Dibromofluoromethane           | S           | ug/L         | 278.46353  | 11.1385412    |                  | 10    | 0        | 0         | 0.129  | 0.5    | 500    | 111% | 77  | 126  | 0%   |   |
| p-Bromofluorobenzene           | S           | ug/L         | 267.28149  | 10.6912596    |                  | 10    | 0        | 0         | 0.149  | 0.5    | 500    | 107% | 76  | 127  | 0%   |   |
| Toluene-d8                     | S           | ug/L         | 265.34358  | 10.6137432    |                  | 10    | 0        | 0         | 0.23   | 0.5    | 500    | 106% | 79  | 122  | 0%   |   |

| Seq No              | Lab ID       | Test Code    | Sample Typ | File ID       | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|---------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970899            | ICAL010422_1 | VOC-8260-W-Q | CAL1       | DA5975C\VG010 | 1/4/2022 3:33:04 | 1     | R372940  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte             | T            | Units        | RAW        | Final         | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| 1,2-Dichlorobenzene | A            | ug/L         | 2.73073    | 0.1092292     |                  | 0.1   | 0        | 0         | 0.0746 | 0.5    | 500    | 109% | 50  | 150  | 0%   |   |
| 1,2-Dichloroethane  | A            | ug/L         | 2.90899    | 0.1163596     |                  | 0.1   | 0        | 0         | 0.116  | 0.5    | 500    | 116% | 50  | 150  | 0%   |   |
| 1,3-Dichlorobenzene | A            | ug/L         | 2.6327     | 0.105308      |                  | 0.1   | 0        | 0         | 0.0803 | 0.5    | 500    | 105% | 50  | 150  | 0%   |   |
| 1,4-Dichlorobenzene | A            | ug/L         | 2.76134    | 0.1104536     |                  | 0.1   | 0        | 0         | 0.0858 | 0.5    | 500    | 110% | 50  | 150  | 0%   |   |
| Benzene             | A            | ug/L         | 2.73933    | 0.1095732     |                  | 0.1   | 0        | 0         | 0.0914 | 0.5    | 500    | 110% | 50  | 150  | 0%   |   |
| Chloroform          | A            | ug/L         | 2.89464    | 0.1157856     |                  | 0.1   | 0        | 0         | 0.0789 | 0.5    | 500    | 116% | 50  | 150  | 0%   |   |
| Ethylbenzene        | A            | ug/L         | 2.53666    | 0.1014664     |                  | 0.1   | 0        | 0         | 0.0836 | 0.5    | 500    | 101% | 50  | 150  | 0%   |   |
| m+p-Xylenes         | A            | ug/L         | 5.07121    | 0.2028484     |                  | 0.2   | 0        | 0         | 0.15   | 0.5    | 1000   | 101% | 50  | 150  | 0%   |   |
| Styrene             | A            | ug/L         | 2.16254    | 0.0865016     |                  | 0.1   | 0        | 0         | 0.067  | 0.5    | 500    | 87%  | 50  | 150  | 0%   |   |

| Seq No                    | Lab ID       | Test Code    | Sample Typ | File ID       | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|---------------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970899                  | ICAL010422_1 | VOC-8260-W-Q | CAL1       | DA5975C\VG010 | 1/4/2022 3:33:04 | 1     | R372940  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                   | T            | Units        | RAW        | Final         | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| Tetrachloroethene         | A            | ug/L         | 2.67723    | 0.1070892     |                  | 0.1   | 0        | 0         | 0.0671 | 0.5    | 500    | 107% | 50  | 150  | 0%   |   |
| Toluene                   | A            | ug/L         | 2.6145     | 0.10458       |                  | 0.1   | 0        | 0         | 0.0679 | 0.5    | 500    | 105% | 50  | 150  | 0%   |   |
| Seq No                    | Lab ID       | Test Code    | Sample Typ | File ID       | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
| 14970901                  | ICAL010422_2 | VOC-8260-W-Q | CAL2       | DA5975C\VG010 | 1/4/2022 4:00:35 | 1     | R372940  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                   | T            | Units        | RAW        | Final         | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A            | ug/L         | 12.82253   | 0.5129012     |                  | 0.5   | 0        | 0         | 0.101  | 0.5    | 500    | 103% | 50  | 150  | 0%   |   |
| 1,1,1-Trichloroethane     | A            | ug/L         | 12.18907   | 0.4875628     |                  | 0.5   | 0        | 0         | 0.131  | 0.5    | 500    | 98%  | 50  | 150  | 0%   |   |
| 1,1,2,2-Tetrachloroethane | A            | ug/L         | 12.84375   | 0.51375       |                  | 0.5   | 0        | 0         | 0.0872 | 0.5    | 500    | 103% | 50  | 150  | 0%   |   |
| 1,1,2-Trichloroethane     | A            | ug/L         | 13.23404   | 0.5293616     |                  | 0.5   | 0        | 0         | 0.108  | 0.5    | 500    | 106% | 50  | 150  | 0%   |   |
| 1,1-Dichloroethane        | A            | ug/L         | 12.06522   | 0.4826088     |                  | 0.5   | 0        | 0         | 0.135  | 0.5    | 500    | 97%  | 50  | 150  | 0%   |   |
| 1,1-Dichloroethene        | A            | ug/L         | 11.90807   | 0.4763228     |                  | 0.5   | 0        | 0         | 0.141  | 0.5    | 500    | 95%  | 50  | 150  | 0%   |   |
| 1,1-Dichloropropene       | A            | ug/L         | 11.33971   | 0.4535884     |                  | 0.5   | 0        | 0         | 0.083  | 0.5    | 500    | 91%  | 50  | 150  | 0%   |   |
| 1,2,3-Trichloropropane    | A            | ug/L         | 13.70838   | 0.5483352     |                  | 0.5   | 0        | 0         | 0.235  | 0.5    | 500    | 110% | 50  | 150  | 0%   |   |
| 1,2-Dibromoethane         | A            | ug/L         | 12.86397   | 0.5145588     |                  | 0.5   | 0        | 0         | 0.0916 | 0.5    | 500    | 103% | 50  | 150  | 0%   |   |
| 1,2-Dichlorobenzene       | A            | ug/L         | 12.14234   | 0.4856936     |                  | 0.5   | 0        | 0         | 0.0746 | 0.5    | 500    | 97%  | 70  | 130  | 0%   |   |
| 1,2-Dichloroethane        | A            | ug/L         | 12.39059   | 0.4956236     |                  | 0.5   | 0        | 0         | 0.116  | 0.5    | 500    | 99%  | 70  | 130  | 0%   |   |
| 1,2-Dichloropropane       | A            | ug/L         | 12.0602    | 0.482408      |                  | 0.5   | 0        | 0         | 0.0847 | 0.5    | 500    | 96%  | 50  | 150  | 0%   |   |
| 1,3-Dichlorobenzene       | A            | ug/L         | 11.84726   | 0.4738904     |                  | 0.5   | 0        | 0         | 0.0803 | 0.5    | 500    | 95%  | 70  | 130  | 0%   |   |
| 1,3-Dichloropropane       | A            | ug/L         | 11.85262   | 0.4741048     |                  | 0.5   | 0        | 0         | 0.0791 | 0.5    | 500    | 95%  | 50  | 150  | 0%   |   |
| 1,4-Dichlorobenzene       | A            | ug/L         | 11.96618   | 0.4786472     |                  | 0.5   | 0        | 0         | 0.0858 | 0.5    | 500    | 96%  | 70  | 130  | 0%   |   |
| 2,2-Dichloropropane       | A            | ug/L         | 12.48201   | 0.4992804     |                  | 0.5   | 0        | 0         | 0.186  | 0.5    | 500    | 100% | 50  | 150  | 0%   |   |
| 2-Chlorotoluene           | A            | ug/L         | 11.19768   | 0.4479072     |                  | 0.5   | 0        | 0         | 0.0876 | 0.5    | 500    | 90%  | 50  | 150  | 0%   |   |
| 4-Chlorotoluene           | A            | ug/L         | 11.22327   | 0.4489308     |                  | 0.5   | 0        | 0         | 0.0728 | 0.5    | 500    | 90%  | 50  | 150  | 0%   |   |
| Benzene                   | A            | ug/L         | 12.18007   | 0.4872028     |                  | 0.5   | 0        | 0         | 0.0914 | 0.5    | 500    | 97%  | 70  | 130  | 0%   |   |
| Bromobenzene              | A            | ug/L         | 12.331     | 0.49324       |                  | 0.5   | 0        | 0         | 0.0831 | 0.5    | 500    | 99%  | 50  | 150  | 0%   |   |
| Bromochloromethane        | A            | ug/L         | 12.9568    | 0.518272      |                  | 0.5   | 0        | 0         | 0.141  | 0.5    | 500    | 104% | 50  | 150  | 0%   |   |
| Bromodichloromethane      | A            | ug/L         | 12.60141   | 0.5040564     |                  | 0.5   | 0        | 0         | 0.12   | 0.5    | 500    | 101% | 50  | 150  | 0%   |   |
| Bromoform                 | A            | ug/L         | 11.78598   | 0.4714392     |                  | 0.5   | 0        | 0         | 0.119  | 0.5    | 500    | 94%  | 50  | 150  | 0%   |   |
| Bromomethane              | A            | ug/L         | 12.04638   | 0.4818552     |                  | 0.5   | 0        | 0         | 0.253  | 0.5    | 500    | 96%  | 50  | 150  | 0%   |   |
| Carbon tetrachloride      | A            | ug/L         | 12.2545    | 0.49018       |                  | 0.5   | 0        | 0         | 0.143  | 0.5    | 500    | 98%  | 50  | 150  | 0%   |   |
| Chlorobenzene             | A            | ug/L         | 12.52043   | 0.5008172     |                  | 0.5   | 0        | 0         | 0.0914 | 0.5    | 500    | 100% | 50  | 150  | 0%   |   |
| Chlorodibromomethane      | A            | ug/L         | 12.83929   | 0.5135716     |                  | 0.5   | 0        | 0         | 0.0841 | 0.5    | 500    | 103% | 50  | 150  | 0%   |   |
| Chloroethane              | A            | ug/L         | 14.86697   | 0.5946788     |                  | 0.5   | 0        | 0         | 0.169  | 0.5    | 500    | 119% | 50  | 150  | 0%   |   |

| Seq No                         | Lab ID       | Test Code    | Sample Typ | File ID       | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|--------------------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970901                       | ICAL010422_2 | VOC-8260-W-Q | CAL2       | DA5975C\VG010 | 1/4/2022 4:00:35 | 1     | R372940  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                        | T            | Units        | RAW        | Final         | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| Chloroform                     | A            | ug/L         | 13.06683   | 0.5226732     |                  | 0.5   | 0        | 0         | 0.0789 | 0.5    | 500    | 105% | 70  | 130  | 0%   |   |
| Chloromethane                  | A            | ug/L         | 13.86612   | 0.5546448     |                  | 0.5   | 0        | 0         | 0.162  | 0.5    | 500    | 111% | 50  | 150  | 0%   |   |
| cis-1,2-Dichloroethene         | A            | ug/L         | 12.56593   | 0.5026372     |                  | 0.5   | 0        | 0         | 0.108  | 0.5    | 500    | 101% | 50  | 150  | 0%   |   |
| cis-1,3-Dichloropropene        | A            | ug/L         | 12.07376   | 0.4829504     |                  | 0.5   | 0        | 0         | 0.073  | 0.5    | 500    | 97%  | 50  | 150  | 0%   |   |
| Dibromomethane                 | A            | ug/L         | 14.06189   | 0.5624756     |                  | 0.5   | 0        | 0         | 0.147  | 0.5    | 500    | 112% | 50  | 150  | 0%   |   |
| Dichlorodifluoromethane        | A            | ug/L         | 12.06625   | 0.48265       |                  | 0.5   | 0        | 0         | 0.175  | 0.5    | 500    | 97%  | 50  | 150  | 0%   |   |
| Ethylbenzene                   | A            | ug/L         | 11.04112   | 0.4416448     |                  | 0.5   | 0        | 0         | 0.0836 | 0.5    | 500    | 88%  | 70  | 130  | 0%   |   |
| m+p-Xylenes                    | A            | ug/L         | 22.14096   | 0.8856384     |                  | 1     | 0        | 0         | 0.15   | 0.5    | 1000   | 89%  | 70  | 130  | 0%   |   |
| Methyl ethyl ketone            | A            | ug/L         | 122.052    | 4.88208       |                  | 5     | 0        | 0         | 1.77   | 10     | 5000   | 98%  | 50  | 150  | 0%   |   |
| Methyl tert-butyl ether (MTBE) | A            | ug/L         | 12.32545   | 0.493018      |                  | 0.5   | 0        | 0         | 0.101  | 0.5    | 500    | 99%  | 50  | 150  | 0%   |   |
| Methylene chloride             | A            | ug/L         | 15.62358   | 0.6249432     |                  | 0.5   | 0        | 0         | 0.338  | 0.5    | 500    | 125% | 50  | 150  | 0%   |   |
| o-Xylene                       | A            | ug/L         | 10.66119   | 0.4264476     |                  | 0.5   | 0        | 0         | 0.0604 | 0.5    | 500    | 85%  | 50  | 150  | 0%   |   |
| Styrene                        | A            | ug/L         | 11.49684   | 0.4598736     |                  | 0.5   | 0        | 0         | 0.067  | 0.5    | 500    | 92%  | 70  | 130  | 0%   |   |
| Tetrachloroethene              | A            | ug/L         | 11.73024   | 0.4692096     |                  | 0.5   | 0        | 0         | 0.0671 | 0.5    | 500    | 94%  | 70  | 130  | 0%   |   |
| Toluene                        | A            | ug/L         | 11.28985   | 0.451594      |                  | 0.5   | 0        | 0         | 0.0679 | 0.5    | 500    | 90%  | 70  | 130  | 0%   |   |
| trans-1,2-Dichloroethene       | A            | ug/L         | 12.50224   | 0.5000896     |                  | 0.5   | 0        | 0         | 0.125  | 0.5    | 500    | 100% | 50  | 150  | 0%   |   |
| trans-1,3-Dichloropropene      | A            | ug/L         | 11.75888   | 0.4703552     |                  | 0.5   | 0        | 0         | 0.0846 | 0.5    | 500    | 94%  | 50  | 150  | 0%   |   |
| Trichloroethene                | A            | ug/L         | 11.67527   | 0.4670108     |                  | 0.5   | 0        | 0         | 0.0993 | 0.5    | 500    | 93%  | 50  | 150  | 0%   |   |
| Trichlorofluoromethane         | A            | ug/L         | 11.36372   | 0.4545488     |                  | 0.5   | 0        | 0         | 0.134  | 0.5    | 500    | 91%  | 50  | 150  | 0%   |   |
| Vinyl chloride                 | A            | ug/L         | 12.54456   | 0.5017824     |                  | 0.5   | 0        | 0         | 0.153  | 0.5    | 500    | 100% | 50  | 150  | 0%   |   |
| 1,4-Dichlorobenzene-d4         | I            | ug/L         | 250        | 10            |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 50  | 150  | 0%   |   |
| Chlorobenzene-d5               | I            | ug/L         | 250        | 10            |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 50  | 150  | 0%   |   |
| Fluorobenzene                  | I            | ug/L         | 250        | 10            |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 50  | 150  | 0%   |   |
| Xylenes, Total                 | M            | ug/L         | 32.80215   | 1.312086      |                  | 1.5   | 0        | 0         | 0.0604 | 0.5    | 1500   | 87%  | 50  | 150  | 0%   |   |
| 1,2-Dichloroethane-d4          | S            | ug/L         | 12.66005   | 0.506402      |                  | 0.5   | 0        | 0         | 0.229  | 0.5    | 500    | 101% | 50  | 150  | 0%   |   |
| Dibromofluoromethane           | S            | ug/L         | 12.59997   | 0.5039988     |                  | 0.5   | 0        | 0         | 0.129  | 0.5    | 500    | 101% | 50  | 150  | 0%   |   |
| p-Bromofluorobenzene           | S            | ug/L         | 11.33932   | 0.4535728     |                  | 0.5   | 0        | 0         | 0.149  | 0.5    | 500    | 91%  | 50  | 150  | 0%   |   |
| Toluene-d8                     | S            | ug/L         | 11.30891   | 0.4523564     |                  | 0.5   | 0        | 0         | 0.23   | 0.5    | 500    | 90%  | 50  | 150  | 0%   |   |

| Seq No   | Lab ID       | Test Code    | Sample Typ | File ID       | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|----------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970902 | ICAL010422_3 | VOC-8260-W-Q | CAL3       | DA5975C\VG010 | 1/4/2022 4:28:05 | 1     | R372940  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte  | T            | Units        | RAW        | Final         | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |

| Seq No                    | Lab ID       | Test Code    | Sample Typ | File ID       | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|---------------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970902                  | ICAL010422_3 | VOC-8260-W-Q | CAL3       | DA5975C\VG010 | 1/4/2022 4:28:05 | 1     | R372940  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                   | T            | Units        | RAW        | Final         | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A            | ug/L         | 24.15093   | 0.9660372     |                  | 1     | 0        | 0         | 0.101  | 0.5    | 500    | 97%  | 70  | 130  | 0%   |   |
| 1,1,1-Trichloroethane     | A            | ug/L         | 25.18087   | 1.0072348     |                  | 1     | 0        | 0         | 0.131  | 0.5    | 500    | 101% | 70  | 130  | 0%   |   |
| 1,1,2,2-Tetrachloroethane | A            | ug/L         | 27.78828   | 1.1115312     |                  | 1     | 0        | 0         | 0.0872 | 0.5    | 500    | 111% | 70  | 130  | 0%   |   |
| 1,1,2-Trichloroethane     | A            | ug/L         | 25.84      | 1.0336        |                  | 1     | 0        | 0         | 0.108  | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| 1,1-Dichloroethane        | A            | ug/L         | 25.68346   | 1.0273384     |                  | 1     | 0        | 0         | 0.135  | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| 1,1-Dichloroethene        | A            | ug/L         | 25.88489   | 1.0353956     |                  | 1     | 0        | 0         | 0.141  | 0.5    | 500    | 104% | 70  | 130  | 0%   |   |
| 1,1-Dichloropropene       | A            | ug/L         | 24.36174   | 0.9744696     |                  | 1     | 0        | 0         | 0.083  | 0.5    | 500    | 97%  | 70  | 130  | 0%   |   |
| 1,2,3-Trichloropropane    | A            | ug/L         | 26.71444   | 1.0685776     |                  | 1     | 0        | 0         | 0.235  | 0.5    | 500    | 107% | 70  | 130  | 0%   |   |
| 1,2-Dibromoethane         | A            | ug/L         | 24.36006   | 0.9744024     |                  | 1     | 0        | 0         | 0.0916 | 0.5    | 500    | 97%  | 70  | 130  | 0%   |   |
| 1,2-Dichlorobenzene       | A            | ug/L         | 24.94023   | 0.9976092     |                  | 1     | 0        | 0         | 0.0746 | 0.5    | 500    | 100% | 70  | 130  | 0%   |   |
| 1,2-Dichloroethane        | A            | ug/L         | 23.46155   | 0.938462      |                  | 1     | 0        | 0         | 0.116  | 0.5    | 500    | 94%  | 70  | 130  | 0%   |   |
| 1,2-Dichloropropane       | A            | ug/L         | 25.11474   | 1.0045896     |                  | 1     | 0        | 0         | 0.0847 | 0.5    | 500    | 100% | 70  | 130  | 0%   |   |
| 1,3-Dichlorobenzene       | A            | ug/L         | 25.77252   | 1.0309008     |                  | 1     | 0        | 0         | 0.0803 | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| 1,3-Dichloropropane       | A            | ug/L         | 24.38386   | 0.9753544     |                  | 1     | 0        | 0         | 0.0791 | 0.5    | 500    | 98%  | 70  | 130  | 0%   |   |
| 1,4-Dichlorobenzene       | A            | ug/L         | 25.32843   | 1.0131372     |                  | 1     | 0        | 0         | 0.0858 | 0.5    | 500    | 101% | 70  | 130  | 0%   |   |
| 2,2-Dichloropropane       | A            | ug/L         | 26.26917   | 1.0507668     |                  | 1     | 0        | 0         | 0.186  | 0.5    | 500    | 105% | 70  | 130  | 0%   |   |
| 2-Chlorotoluene           | A            | ug/L         | 25.05504   | 1.0022016     |                  | 1     | 0        | 0         | 0.0876 | 0.5    | 500    | 100% | 70  | 130  | 0%   |   |
| 4-Chlorotoluene           | A            | ug/L         | 24.39357   | 0.9757428     |                  | 1     | 0        | 0         | 0.0728 | 0.5    | 500    | 98%  | 70  | 130  | 0%   |   |
| Benzene                   | A            | ug/L         | 23.79187   | 0.9516748     |                  | 1     | 0        | 0         | 0.0914 | 0.5    | 500    | 95%  | 70  | 130  | 0%   |   |
| Bromobenzene              | A            | ug/L         | 24.76128   | 0.9904512     |                  | 1     | 0        | 0         | 0.0831 | 0.5    | 500    | 99%  | 70  | 130  | 0%   |   |
| Bromochloromethane        | A            | ug/L         | 25.4383    | 1.017532      |                  | 1     | 0        | 0         | 0.141  | 0.5    | 500    | 102% | 70  | 130  | 0%   |   |
| Bromodichloromethane      | A            | ug/L         | 24.39404   | 0.9757616     |                  | 1     | 0        | 0         | 0.12   | 0.5    | 500    | 98%  | 70  | 130  | 0%   |   |
| Bromoform                 | A            | ug/L         | 25.92121   | 1.0368484     |                  | 1     | 0        | 0         | 0.119  | 0.5    | 500    | 104% | 70  | 130  | 0%   |   |
| Bromomethane              | A            | ug/L         | 25.77927   | 1.0311708     |                  | 1     | 0        | 0         | 0.253  | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| Carbon tetrachloride      | A            | ug/L         | 24.77733   | 0.9910932     |                  | 1     | 0        | 0         | 0.143  | 0.5    | 500    | 99%  | 70  | 130  | 0%   |   |
| Chlorobenzene             | A            | ug/L         | 24.70152   | 0.9880608     |                  | 1     | 0        | 0         | 0.0914 | 0.5    | 500    | 99%  | 70  | 130  | 0%   |   |
| Chlorodibromomethane      | A            | ug/L         | 24.3492    | 0.973968      |                  | 1     | 0        | 0         | 0.0841 | 0.5    | 500    | 97%  | 70  | 130  | 0%   |   |
| Chloroethane              | A            | ug/L         | 26.12501   | 1.0450004     |                  | 1     | 0        | 0         | 0.169  | 0.5    | 500    | 105% | 70  | 130  | 0%   |   |
| Chloroform                | A            | ug/L         | 24.17337   | 0.9669348     |                  | 1     | 0        | 0         | 0.0789 | 0.5    | 500    | 97%  | 70  | 130  | 0%   |   |
| Chloromethane             | A            | ug/L         | 26.34224   | 1.0536896     |                  | 1     | 0        | 0         | 0.162  | 0.5    | 500    | 105% | 70  | 130  | 0%   |   |
| cis-1,2-Dichloroethene    | A            | ug/L         | 24.5653    | 0.982612      |                  | 1     | 0        | 0         | 0.108  | 0.5    | 500    | 98%  | 70  | 130  | 0%   |   |
| cis-1,3-Dichloropropene   | A            | ug/L         | 23.25283   | 0.9301132     |                  | 1     | 0        | 0         | 0.073  | 0.5    | 500    | 93%  | 70  | 130  | 0%   |   |
| Dibromomethane            | A            | ug/L         | 23.84392   | 0.9537568     |                  | 1     | 0        | 0         | 0.147  | 0.5    | 500    | 95%  | 70  | 130  | 0%   |   |
| Dichlorodifluoromethane   | A            | ug/L         | 25.67929   | 1.0271716     |                  | 1     | 0        | 0         | 0.175  | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| Ethylbenzene              | A            | ug/L         | 23.74212   | 0.9496848     |                  | 1     | 0        | 0         | 0.0836 | 0.5    | 500    | 95%  | 70  | 130  | 0%   |   |

| Seq No                         | Lab ID       | Test Code    | Sample Typ | File ID       | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|--------------------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970902                       | ICAL010422_3 | VOC-8260-W-Q | CAL3       | DA5975C\VG010 | 1/4/2022 4:28:05 | 1     | R372940  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                        | T            | Units        | RAW        | Final         | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| m+p-Xylenes                    | A            | ug/L         | 45.78355   | 1.831342      |                  | 2     | 0        | 0         | 0.15   | 0.5    | 1000   | 92%  | 70  | 130  | 0%   |   |
| Methyl ethyl ketone            | A            | ug/L         | 235.05043  | 9.4020172     |                  | 10    | 0        | 0         | 1.77   | 10     | 5000   | 94%  | 70  | 130  | 0%   |   |
| Methyl tert-butyl ether (MTBE) | A            | ug/L         | 23.04184   | 0.9216736     |                  | 1     | 0        | 0         | 0.101  | 0.5    | 500    | 92%  | 70  | 130  | 0%   |   |
| Methylene chloride             | A            | ug/L         | 26.30581   | 1.0522324     |                  | 1     | 0        | 0         | 0.338  | 0.5    | 500    | 105% | 70  | 130  | 0%   |   |
| o-Xylene                       | A            | ug/L         | 23.64197   | 0.9456788     |                  | 1     | 0        | 0         | 0.0604 | 0.5    | 500    | 95%  | 70  | 130  | 0%   |   |
| Styrene                        | A            | ug/L         | 23.41194   | 0.9364776     |                  | 1     | 0        | 0         | 0.067  | 0.5    | 500    | 94%  | 70  | 130  | 0%   |   |
| Tetrachloroethene              | A            | ug/L         | 25.39483   | 1.0157932     |                  | 1     | 0        | 0         | 0.0671 | 0.5    | 500    | 102% | 70  | 130  | 0%   |   |
| Toluene                        | A            | ug/L         | 23.63186   | 0.9452744     |                  | 1     | 0        | 0         | 0.0679 | 0.5    | 500    | 95%  | 70  | 130  | 0%   |   |
| trans-1,2-Dichloroethene       | A            | ug/L         | 25.46407   | 1.0185628     |                  | 1     | 0        | 0         | 0.125  | 0.5    | 500    | 102% | 70  | 130  | 0%   |   |
| trans-1,3-Dichloropropene      | A            | ug/L         | 23.78943   | 0.9515772     |                  | 1     | 0        | 0         | 0.0846 | 0.5    | 500    | 95%  | 70  | 130  | 0%   |   |
| Trichloroethene                | A            | ug/L         | 24.14841   | 0.9659364     |                  | 1     | 0        | 0         | 0.0993 | 0.5    | 500    | 97%  | 70  | 130  | 0%   |   |
| Trichlorofluoromethane         | A            | ug/L         | 26.65307   | 1.0661228     |                  | 1     | 0        | 0         | 0.134  | 0.5    | 500    | 107% | 70  | 130  | 0%   |   |
| Vinyl chloride                 | A            | ug/L         | 25.64884   | 1.0259536     |                  | 1     | 0        | 0         | 0.153  | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| 1,4-Dichlorobenzene-d4         | I            | ug/L         | 250        | 10            |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 70  | 130  | 0%   |   |
| Chlorobenzene-d5               | I            | ug/L         | 250        | 10            |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 70  | 130  | 0%   |   |
| Fluorobenzene                  | I            | ug/L         | 250        | 10            |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 70  | 130  | 0%   |   |
| Xylenes, Total                 | M            | ug/L         | 69.42552   | 2.7770208     |                  | 3     | 0        | 0         | 0.0604 | 0.5    | 1500   | 93%  | 70  | 130  | 0%   |   |
| 1,2-Dichloroethane-d4          | S            | ug/L         | 25.72803   | 1.0291212     |                  | 1     | 0        | 0         | 0.229  | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| Dibromofluoromethane           | S            | ug/L         | 25.62188   | 1.0248752     |                  | 1     | 0        | 0         | 0.129  | 0.5    | 500    | 102% | 70  | 130  | 0%   |   |
| p-Bromofluorobenzene           | S            | ug/L         | 25.28989   | 1.0115956     |                  | 1     | 0        | 0         | 0.149  | 0.5    | 500    | 101% | 70  | 130  | 0%   |   |
| Toluene-d8                     | S            | ug/L         | 23.3046    | 0.932184      |                  | 1     | 0        | 0         | 0.23   | 0.5    | 500    | 93%  | 70  | 130  | 0%   |   |

| Seq No                    | Lab ID       | Test Code    | Sample Typ | File ID       | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|---------------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970904                  | ICAL010422_4 | VOC-8260-W-Q | CAL4       | DA5975C\VG010 | 1/4/2022 4:55:32 | 1     | R372940  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                   | T            | Units        | RAW        | Final         | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A            | ug/L         | 47.50287   | 1.9001148     |                  | 2     | 0        | 0         | 0.101  | 0.5    | 500    | 95%  | 70  | 130  | 0%   |   |
| 1,1,1-Trichloroethane     | A            | ug/L         | 48.26875   | 1.93075       |                  | 2     | 0        | 0         | 0.131  | 0.5    | 500    | 97%  | 70  | 130  | 0%   |   |
| 1,1,2,2-Tetrachloroethane | A            | ug/L         | 48.61239   | 1.9444956     |                  | 2     | 0        | 0         | 0.0872 | 0.5    | 500    | 97%  | 70  | 130  | 0%   |   |
| 1,1,2-Trichloroethane     | A            | ug/L         | 48.47589   | 1.9390356     |                  | 2     | 0        | 0         | 0.108  | 0.5    | 500    | 97%  | 70  | 130  | 0%   |   |
| 1,1-Dichloroethane        | A            | ug/L         | 49.18279   | 1.9673116     |                  | 2     | 0        | 0         | 0.135  | 0.5    | 500    | 98%  | 70  | 130  | 0%   |   |
| 1,1-Dichloroethene        | A            | ug/L         | 48.80561   | 1.9522244     |                  | 2     | 0        | 0         | 0.141  | 0.5    | 500    | 98%  | 70  | 130  | 0%   |   |
| 1,1-Dichloropropene       | A            | ug/L         | 47.76266   | 1.9105064     |                  | 2     | 0        | 0         | 0.083  | 0.5    | 500    | 96%  | 70  | 130  | 0%   |   |
| 1,2,3-Trichloropropane    | A            | ug/L         | 49.19244   | 1.9676976     |                  | 2     | 0        | 0         | 0.235  | 0.5    | 500    | 98%  | 70  | 130  | 0%   |   |
| 1,2-Dibromoethane         | A            | ug/L         | 49.38886   | 1.9755544     |                  | 2     | 0        | 0         | 0.0916 | 0.5    | 500    | 99%  | 70  | 130  | 0%   |   |

| Seq No                         | Lab ID       | Test Code    | Sample Typ | File ID       | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|--------------------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970904                       | ICAL010422_4 | VOC-8260-W-Q | CAL4       | DA5975C\VG010 | 1/4/2022 4:55:32 | 1     | R372940  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                        | T            | Units        | RAW        | Final         | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| 1,2-Dichlorobenzene            | A            | ug/L         | 48.54976   | 1.9419904     |                  | 2     | 0        | 0         | 0.0746 | 0.5    | 500    | 97%  | 70  | 130  | 0%   |   |
| 1,2-Dichloroethane             | A            | ug/L         | 48.98798   | 1.9595192     |                  | 2     | 0        | 0         | 0.116  | 0.5    | 500    | 98%  | 70  | 130  | 0%   |   |
| 1,2-Dichloropropane            | A            | ug/L         | 47.52725   | 1.90109       |                  | 2     | 0        | 0         | 0.0847 | 0.5    | 500    | 95%  | 70  | 130  | 0%   |   |
| 1,3-Dichlorobenzene            | A            | ug/L         | 47.38535   | 1.895414      |                  | 2     | 0        | 0         | 0.0803 | 0.5    | 500    | 95%  | 70  | 130  | 0%   |   |
| 1,3-Dichloropropane            | A            | ug/L         | 48.8841    | 1.955364      |                  | 2     | 0        | 0         | 0.0791 | 0.5    | 500    | 98%  | 70  | 130  | 0%   |   |
| 1,4-Dichlorobenzene            | A            | ug/L         | 48.01064   | 1.9204256     |                  | 2     | 0        | 0         | 0.0858 | 0.5    | 500    | 96%  | 70  | 130  | 0%   |   |
| 2,2-Dichloropropane            | A            | ug/L         | 50.38039   | 2.0152156     |                  | 2     | 0        | 0         | 0.186  | 0.5    | 500    | 101% | 70  | 130  | 0%   |   |
| 2-Chlorotoluene                | A            | ug/L         | 47.44663   | 1.8978652     |                  | 2     | 0        | 0         | 0.0876 | 0.5    | 500    | 95%  | 70  | 130  | 0%   |   |
| 4-Chlorotoluene                | A            | ug/L         | 48.3865    | 1.93546       |                  | 2     | 0        | 0         | 0.0728 | 0.5    | 500    | 97%  | 70  | 130  | 0%   |   |
| Benzene                        | A            | ug/L         | 48.00539   | 1.9202156     |                  | 2     | 0        | 0         | 0.0914 | 0.5    | 500    | 96%  | 70  | 130  | 0%   |   |
| Bromobenzene                   | A            | ug/L         | 47.5759    | 1.903036      |                  | 2     | 0        | 0         | 0.0831 | 0.5    | 500    | 95%  | 70  | 130  | 0%   |   |
| Bromochloromethane             | A            | ug/L         | 51.62325   | 2.06493       |                  | 2     | 0        | 0         | 0.141  | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| Bromodichloromethane           | A            | ug/L         | 47.2409    | 1.889636      |                  | 2     | 0        | 0         | 0.12   | 0.5    | 500    | 94%  | 70  | 130  | 0%   |   |
| Bromoform                      | A            | ug/L         | 50.51704   | 2.0206816     |                  | 2     | 0        | 0         | 0.119  | 0.5    | 500    | 101% | 70  | 130  | 0%   |   |
| Bromomethane                   | A            | ug/L         | 47.59212   | 1.9036848     |                  | 2     | 0        | 0         | 0.253  | 0.5    | 500    | 95%  | 70  | 130  | 0%   |   |
| Carbon tetrachloride           | A            | ug/L         | 47.75203   | 1.9100812     |                  | 2     | 0        | 0         | 0.143  | 0.5    | 500    | 96%  | 70  | 130  | 0%   |   |
| Chlorobenzene                  | A            | ug/L         | 47.39593   | 1.8958372     |                  | 2     | 0        | 0         | 0.0914 | 0.5    | 500    | 95%  | 70  | 130  | 0%   |   |
| Chlorodibromomethane           | A            | ug/L         | 46.24113   | 1.8496452     |                  | 2     | 0        | 0         | 0.0841 | 0.5    | 500    | 92%  | 70  | 130  | 0%   |   |
| Chloroethane                   | A            | ug/L         | 46.22429   | 1.8489716     |                  | 2     | 0        | 0         | 0.169  | 0.5    | 500    | 92%  | 70  | 130  | 0%   |   |
| Chloroform                     | A            | ug/L         | 48.20314   | 1.9281256     |                  | 2     | 0        | 0         | 0.0789 | 0.5    | 500    | 96%  | 70  | 130  | 0%   |   |
| Chloromethane                  | A            | ug/L         | 49.79828   | 1.9919312     |                  | 2     | 0        | 0         | 0.162  | 0.5    | 500    | 100% | 70  | 130  | 0%   |   |
| cis-1,2-Dichloroethene         | A            | ug/L         | 48.41535   | 1.936614      |                  | 2     | 0        | 0         | 0.108  | 0.5    | 500    | 97%  | 70  | 130  | 0%   |   |
| cis-1,3-Dichloropropene        | A            | ug/L         | 46.52826   | 1.8611304     |                  | 2     | 0        | 0         | 0.073  | 0.5    | 500    | 93%  | 70  | 130  | 0%   |   |
| Dibromomethane                 | A            | ug/L         | 47.4844    | 1.899376      |                  | 2     | 0        | 0         | 0.147  | 0.5    | 500    | 95%  | 70  | 130  | 0%   |   |
| Dichlorodifluoromethane        | A            | ug/L         | 49.48348   | 1.9793392     |                  | 2     | 0        | 0         | 0.175  | 0.5    | 500    | 99%  | 70  | 130  | 0%   |   |
| Ethylbenzene                   | A            | ug/L         | 46.80795   | 1.872318      |                  | 2     | 0        | 0         | 0.0836 | 0.5    | 500    | 94%  | 70  | 130  | 0%   |   |
| m+p-Xylenes                    | A            | ug/L         | 92.53468   | 3.7013872     |                  | 4     | 0        | 0         | 0.15   | 0.5    | 1000   | 93%  | 70  | 130  | 0%   |   |
| Methyl ethyl ketone            | A            | ug/L         | 479.42958  | 19.1771832    |                  | 20    | 0        | 0         | 1.77   | 10     | 5000   | 96%  | 70  | 130  | 0%   |   |
| Methyl tert-butyl ether (MTBE) | A            | ug/L         | 47.53006   | 1.9012024     |                  | 2     | 0        | 0         | 0.101  | 0.5    | 500    | 95%  | 70  | 130  | 0%   |   |
| Methylene chloride             | A            | ug/L         | 50.44212   | 2.0176848     |                  | 2     | 0        | 0         | 0.338  | 0.5    | 500    | 101% | 70  | 130  | 0%   |   |
| o-Xylene                       | A            | ug/L         | 47.5086    | 1.900344      |                  | 2     | 0        | 0         | 0.0604 | 0.5    | 500    | 95%  | 70  | 130  | 0%   |   |
| Styrene                        | A            | ug/L         | 46.70518   | 1.8682072     |                  | 2     | 0        | 0         | 0.067  | 0.5    | 500    | 93%  | 70  | 130  | 0%   |   |
| Tetrachloroethene              | A            | ug/L         | 46.29317   | 1.8517268     |                  | 2     | 0        | 0         | 0.0671 | 0.5    | 500    | 93%  | 70  | 130  | 0%   |   |
| Toluene                        | A            | ug/L         | 47.01163   | 1.8804652     |                  | 2     | 0        | 0         | 0.0679 | 0.5    | 500    | 94%  | 70  | 130  | 0%   |   |
| trans-1,2-Dichloroethene       | A            | ug/L         | 49.51777   | 1.9807108     |                  | 2     | 0        | 0         | 0.125  | 0.5    | 500    | 99%  | 70  | 130  | 0%   |   |



| Seq No                    | Lab ID       | Test Code    | Sample Typ | File ID       | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|---------------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970904                  | ICAL010422_4 | VOC-8260-W-Q | CAL4       | DA5975C\VG010 | 1/4/2022 4:55:32 | 1     | R372940  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                   | T            | Units        | RAW        | Final         | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| trans-1,3-Dichloropropene | A            | ug/L         | 47.0378    | 1.881512      |                  | 2     | 0        | 0         | 0.0846 | 0.5    | 500    | 94%  | 70  | 130  | 0%   |   |
| Trichloroethene           | A            | ug/L         | 47.11894   | 1.8847576     |                  | 2     | 0        | 0         | 0.0993 | 0.5    | 500    | 94%  | 70  | 130  | 0%   |   |
| Trichlorofluoromethane    | A            | ug/L         | 49.31283   | 1.9725132     |                  | 2     | 0        | 0         | 0.134  | 0.5    | 500    | 99%  | 70  | 130  | 0%   |   |
| Vinyl chloride            | A            | ug/L         | 48.95796   | 1.9583184     |                  | 2     | 0        | 0         | 0.153  | 0.5    | 500    | 98%  | 70  | 130  | 0%   |   |
| 1,4-Dichlorobenzene-d4    | I            | ug/L         | 250        | 10            |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 70  | 130  | 0%   |   |
| Chlorobenzene-d5          | I            | ug/L         | 250        | 10            |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 70  | 130  | 0%   |   |
| Fluorobenzene             | I            | ug/L         | 250        | 10            |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 70  | 130  | 0%   |   |
| Xylenes, Total            | M            | ug/L         | 140.04328  | 5.6017312     |                  | 6     | 0        | 0         | 0.0604 | 0.5    | 1500   | 93%  | 70  | 130  | 0%   |   |
| 1,2-Dichloroethane-d4     | S            | ug/L         | 48.12519   | 1.9250076     |                  | 2     | 0        | 0         | 0.229  | 0.5    | 500    | 96%  | 70  | 130  | 0%   |   |
| Dibromofluoromethane      | S            | ug/L         | 48.16607   | 1.9266428     |                  | 2     | 0        | 0         | 0.129  | 0.5    | 500    | 96%  | 70  | 130  | 0%   |   |
| p-Bromofluorobenzene      | S            | ug/L         | 46.6647    | 1.866588      |                  | 2     | 0        | 0         | 0.149  | 0.5    | 500    | 93%  | 70  | 130  | 0%   |   |
| Toluene-d8                | S            | ug/L         | 47.14406   | 1.8857624     |                  | 2     | 0        | 0         | 0.23   | 0.5    | 500    | 94%  | 70  | 130  | 0%   |   |

| Seq No                    | Lab ID       | Test Code    | Sample Typ | File ID       | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|---------------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970905                  | ICAL010422_5 | VOC-8260-W-Q | CAL5       | DA5975C\VG010 | 1/4/2022 5:50:25 | 1     | R372940  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                   | T            | Units        | RAW        | Final         | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A            | ug/L         | 119.0492   | 4.761968      |                  | 5     | 0        | 0         | 0.101  | 0.5    | 500    | 95%  | 70  | 130  | 0%   |   |
| 1,1,1-Trichloroethane     | A            | ug/L         | 118.57641  | 4.7430564     |                  | 5     | 0        | 0         | 0.131  | 0.5    | 500    | 95%  | 70  | 130  | 0%   |   |
| 1,1,2,2-Tetrachloroethane | A            | ug/L         | 115.61793  | 4.6247172     |                  | 5     | 0        | 0         | 0.0872 | 0.5    | 500    | 92%  | 70  | 130  | 0%   |   |
| 1,1,2-Trichloroethane     | A            | ug/L         | 117.41297  | 4.6965188     |                  | 5     | 0        | 0         | 0.108  | 0.5    | 500    | 94%  | 70  | 130  | 0%   |   |
| 1,1-Dichloroethane        | A            | ug/L         | 118.11254  | 4.7245016     |                  | 5     | 0        | 0         | 0.135  | 0.5    | 500    | 94%  | 70  | 130  | 0%   |   |
| 1,1-Dichloroethene        | A            | ug/L         | 119.87977  | 4.7951908     |                  | 5     | 0        | 0         | 0.141  | 0.5    | 500    | 96%  | 70  | 130  | 0%   |   |
| 1,1-Dichloropropene       | A            | ug/L         | 119.80016  | 4.7920064     |                  | 5     | 0        | 0         | 0.083  | 0.5    | 500    | 96%  | 70  | 130  | 0%   |   |
| 1,2,3-Trichloropropane    | A            | ug/L         | 112.62609  | 4.5050436     |                  | 5     | 0        | 0         | 0.235  | 0.5    | 500    | 90%  | 70  | 130  | 0%   |   |
| 1,2-Dibromoethane         | A            | ug/L         | 119.23942  | 4.7695768     |                  | 5     | 0        | 0         | 0.0916 | 0.5    | 500    | 95%  | 70  | 130  | 0%   |   |
| 1,2-Dichlorobenzene       | A            | ug/L         | 115.43227  | 4.6172908     |                  | 5     | 0        | 0         | 0.0746 | 0.5    | 500    | 92%  | 70  | 130  | 0%   |   |
| 1,2-Dichloroethane        | A            | ug/L         | 118.21434  | 4.7285736     |                  | 5     | 0        | 0         | 0.116  | 0.5    | 500    | 95%  | 70  | 130  | 0%   |   |
| 1,2-Dichloropropane       | A            | ug/L         | 121.98902  | 4.8795608     |                  | 5     | 0        | 0         | 0.0847 | 0.5    | 500    | 98%  | 70  | 130  | 0%   |   |
| 1,3-Dichlorobenzene       | A            | ug/L         | 117.4899   | 4.699596      |                  | 5     | 0        | 0         | 0.0803 | 0.5    | 500    | 94%  | 70  | 130  | 0%   |   |
| 1,3-Dichloropropane       | A            | ug/L         | 123.01316  | 4.9205264     |                  | 5     | 0        | 0         | 0.0791 | 0.5    | 500    | 98%  | 70  | 130  | 0%   |   |
| 1,4-Dichlorobenzene       | A            | ug/L         | 118.7699   | 4.750796      |                  | 5     | 0        | 0         | 0.0858 | 0.5    | 500    | 95%  | 70  | 130  | 0%   |   |
| 2,2-Dichloropropane       | A            | ug/L         | 118.32027  | 4.7328108     |                  | 5     | 0        | 0         | 0.186  | 0.5    | 500    | 95%  | 70  | 130  | 0%   |   |
| 2-Chlorotoluene           | A            | ug/L         | 120.26748  | 4.8106992     |                  | 5     | 0        | 0         | 0.0876 | 0.5    | 500    | 96%  | 70  | 130  | 0%   |   |
| 4-Chlorotoluene           | A            | ug/L         | 121.05908  | 4.8423632     |                  | 5     | 0        | 0         | 0.0728 | 0.5    | 500    | 97%  | 70  | 130  | 0%   |   |

| Seq No                         | Lab ID       | Test Code    | Sample Typ | File ID      | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|--------------------------------|--------------|--------------|------------|--------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970905                       | ICAL010422_5 | VOC-8260-W-Q | CAL5       | DA5975CVG010 | 1/4/2022 5:50:25 | 1     | R372940  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                        | T            | Units        | RAW        | Final        | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| Benzene                        | A            | ug/L         | 116.95526  | 4.6782104    |                  | 5     | 0        | 0         | 0.0914 | 0.5    | 500    | 94%  | 70  | 130  | 0%   |   |
| Bromobenzene                   | A            | ug/L         | 119.48008  | 4.7792032    |                  | 5     | 0        | 0         | 0.0831 | 0.5    | 500    | 96%  | 70  | 130  | 0%   |   |
| Bromochloromethane             | A            | ug/L         | 118.06829  | 4.7227316    |                  | 5     | 0        | 0         | 0.141  | 0.5    | 500    | 94%  | 70  | 130  | 0%   |   |
| Bromodichloromethane           | A            | ug/L         | 121.97488  | 4.8789952    |                  | 5     | 0        | 0         | 0.12   | 0.5    | 500    | 98%  | 70  | 130  | 0%   |   |
| Bromoform                      | A            | ug/L         | 115.7218   | 4.628872     |                  | 5     | 0        | 0         | 0.119  | 0.5    | 500    | 93%  | 70  | 130  | 0%   |   |
| Bromomethane                   | A            | ug/L         | 123.65037  | 4.9460148    |                  | 5     | 0        | 0         | 0.253  | 0.5    | 500    | 99%  | 70  | 130  | 0%   |   |
| Carbon tetrachloride           | A            | ug/L         | 119.4667   | 4.778668     |                  | 5     | 0        | 0         | 0.143  | 0.5    | 500    | 96%  | 70  | 130  | 0%   |   |
| Chlorobenzene                  | A            | ug/L         | 120.69031  | 4.8276124    |                  | 5     | 0        | 0         | 0.0914 | 0.5    | 500    | 97%  | 70  | 130  | 0%   |   |
| Chlorodibromomethane           | A            | ug/L         | 120.74537  | 4.8298148    |                  | 5     | 0        | 0         | 0.0841 | 0.5    | 500    | 97%  | 70  | 130  | 0%   |   |
| Chloroethane                   | A            | ug/L         | 122.40855  | 4.896342     |                  | 5     | 0        | 0         | 0.169  | 0.5    | 500    | 98%  | 70  | 130  | 0%   |   |
| Chloroform                     | A            | ug/L         | 114.59119  | 4.5836476    |                  | 5     | 0        | 0         | 0.0789 | 0.5    | 500    | 92%  | 70  | 130  | 0%   |   |
| Chloromethane                  | A            | ug/L         | 122.61785  | 4.904714     |                  | 5     | 0        | 0         | 0.162  | 0.5    | 500    | 98%  | 70  | 130  | 0%   |   |
| cis-1,2-Dichloroethene         | A            | ug/L         | 116.61895  | 4.664758     |                  | 5     | 0        | 0         | 0.108  | 0.5    | 500    | 93%  | 70  | 130  | 0%   |   |
| cis-1,3-Dichloropropene        | A            | ug/L         | 120.71159  | 4.8284636    |                  | 5     | 0        | 0         | 0.073  | 0.5    | 500    | 97%  | 70  | 130  | 0%   |   |
| Dibromomethane                 | A            | ug/L         | 118.24252  | 4.7297008    |                  | 5     | 0        | 0         | 0.147  | 0.5    | 500    | 95%  | 70  | 130  | 0%   |   |
| Dichlorodifluoromethane        | A            | ug/L         | 127.81927  | 5.1127708    |                  | 5     | 0        | 0         | 0.175  | 0.5    | 500    | 102% | 70  | 130  | 0%   |   |
| Ethylbenzene                   | A            | ug/L         | 122.52434  | 4.9009736    |                  | 5     | 0        | 0         | 0.0836 | 0.5    | 500    | 98%  | 70  | 130  | 0%   |   |
| m+p-Xylenes                    | A            | ug/L         | 250.25869  | 10.0103476   |                  | 10    | 0        | 0         | 0.15   | 0.5    | 1000   | 100% | 70  | 130  | 0%   |   |
| Methyl ethyl ketone            | A            | ug/L         | 1159.30194 | 46.3720776   |                  | 50    | 0        | 0         | 1.77   | 10     | 5000   | 93%  | 70  | 130  | 0%   |   |
| Methyl tert-butyl ether (MTBE) | A            | ug/L         | 127.13745  | 5.085498     |                  | 5     | 0        | 0         | 0.101  | 0.5    | 500    | 102% | 70  | 130  | 0%   |   |
| Methylene chloride             | A            | ug/L         | 110.6249   | 4.424996     |                  | 5     | 0        | 0         | 0.338  | 0.5    | 500    | 88%  | 70  | 130  | 0%   |   |
| o-Xylene                       | A            | ug/L         | 123.23778  | 4.9295112    |                  | 5     | 0        | 0         | 0.0604 | 0.5    | 500    | 99%  | 70  | 130  | 0%   |   |
| Styrene                        | A            | ug/L         | 127.19102  | 5.0876408    |                  | 5     | 0        | 0         | 0.067  | 0.5    | 500    | 102% | 70  | 130  | 0%   |   |
| Tetrachloroethene              | A            | ug/L         | 119.90031  | 4.7960124    |                  | 5     | 0        | 0         | 0.0671 | 0.5    | 500    | 96%  | 70  | 130  | 0%   |   |
| Toluene                        | A            | ug/L         | 122.65711  | 4.9062844    |                  | 5     | 0        | 0         | 0.0679 | 0.5    | 500    | 98%  | 70  | 130  | 0%   |   |
| trans-1,2-Dichloroethene       | A            | ug/L         | 118.65107  | 4.7460428    |                  | 5     | 0        | 0         | 0.125  | 0.5    | 500    | 95%  | 70  | 130  | 0%   |   |
| trans-1,3-Dichloropropene      | A            | ug/L         | 121.49288  | 4.8597152    |                  | 5     | 0        | 0         | 0.0846 | 0.5    | 500    | 97%  | 70  | 130  | 0%   |   |
| Trichloroethene                | A            | ug/L         | 123.46463  | 4.9385852    |                  | 5     | 0        | 0         | 0.0993 | 0.5    | 500    | 99%  | 70  | 130  | 0%   |   |
| Trichlorofluoromethane         | A            | ug/L         | 129.06871  | 5.1627484    |                  | 5     | 0        | 0         | 0.134  | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| Vinyl chloride                 | A            | ug/L         | 125.88087  | 5.0352348    |                  | 5     | 0        | 0         | 0.153  | 0.5    | 500    | 101% | 70  | 130  | 0%   |   |
| 1,4-Dichlorobenzene-d4         | I            | ug/L         | 250        | 10           |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 70  | 130  | 0%   |   |
| Chlorobenzene-d5               | I            | ug/L         | 250        | 10           |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 70  | 130  | 0%   |   |
| Fluorobenzene                  | I            | ug/L         | 250        | 10           |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 70  | 130  | 0%   |   |
| Xylenes, Total                 | M            | ug/L         | 373.49647  | 14.9398588   |                  | 15    | 0        | 0         | 0.0604 | 0.5    | 1500   | 100% | 70  | 130  | 0%   |   |
| 1,2-Dichloroethane-d4          | S            | ug/L         | 116.64203  | 4.6656812    |                  | 5     | 0        | 0         | 0.229  | 0.5    | 500    | 93%  | 70  | 130  | 0%   |   |

| Seq No               | Lab ID       | Test Code    | Sample Typ | File ID       | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|----------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970905             | ICAL010422_5 | VOC-8260-W-Q | CAL5       | DA5975C\VG010 | 1/4/2022 5:50:25 | 1     | R372940  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte              | T            | Units        | RAW        | Final         | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| Dibromofluoromethane | S            | ug/L         | 115.11464  | 4.6045856     |                  | 5     | 0        | 0         | 0.129  | 0.5    | 500    | 92%  | 70  | 130  | 0%   |   |
| p-Bromofluorobenzene | S            | ug/L         | 117.93503  | 4.7174012     |                  | 5     | 0        | 0         | 0.149  | 0.5    | 500    | 94%  | 70  | 130  | 0%   |   |
| Toluene-d8           | S            | ug/L         | 121.27495  | 4.850998      |                  | 5     | 0        | 0         | 0.23   | 0.5    | 500    | 97%  | 70  | 130  | 0%   |   |

| Seq No                    | Lab ID       | Test Code    | Sample Typ | File ID       | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|---------------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970906                  | ICAL010422_6 | VOC-8260-W-Q | CAL6       | DA5975C\VG010 | 1/4/2022 6:45:10 | 1     | R372940  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                   | T            | Units        | RAW        | Final         | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A            | ug/L         | 254.82737  | 10.1930948    |                  | 10    | 0        | 0         | 0.101  | 0.5    | 500    | 102% | 70  | 130  | 0%   |   |
| 1,1,1-Trichloroethane     | A            | ug/L         | 258.72281  | 10.3489124    |                  | 10    | 0        | 0         | 0.131  | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| 1,1,2,2-Tetrachloroethane | A            | ug/L         | 250.15769  | 10.0063076    |                  | 10    | 0        | 0         | 0.0872 | 0.5    | 500    | 100% | 70  | 130  | 0%   |   |
| 1,1,2-Trichloroethane     | A            | ug/L         | 248.28816  | 9.9315264     |                  | 10    | 0        | 0         | 0.108  | 0.5    | 500    | 99%  | 70  | 130  | 0%   |   |
| 1,1-Dichloroethane        | A            | ug/L         | 258.43252  | 10.3373008    |                  | 10    | 0        | 0         | 0.135  | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| 1,1-Dichloroethene        | A            | ug/L         | 258.09028  | 10.3236112    |                  | 10    | 0        | 0         | 0.141  | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| 1,1-Dichloropropene       | A            | ug/L         | 264.6638   | 10.586552     |                  | 10    | 0        | 0         | 0.083  | 0.5    | 500    | 106% | 70  | 130  | 0%   |   |
| 1,2,3-Trichloropropane    | A            | ug/L         | 249.26347  | 9.9705388     |                  | 10    | 0        | 0         | 0.235  | 0.5    | 500    | 100% | 70  | 130  | 0%   |   |
| 1,2-Dibromoethane         | A            | ug/L         | 257.88869  | 10.3155476    |                  | 10    | 0        | 0         | 0.0916 | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| 1,2-Dichlorobenzene       | A            | ug/L         | 257.65242  | 10.3060968    |                  | 10    | 0        | 0         | 0.0746 | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| 1,2-Dichloroethane        | A            | ug/L         | 251.96754  | 10.0787016    |                  | 10    | 0        | 0         | 0.116  | 0.5    | 500    | 101% | 70  | 130  | 0%   |   |
| 1,2-Dichloropropane       | A            | ug/L         | 254.71606  | 10.1886424    |                  | 10    | 0        | 0         | 0.0847 | 0.5    | 500    | 102% | 70  | 130  | 0%   |   |
| 1,3-Dichlorobenzene       | A            | ug/L         | 258.62971  | 10.3451884    |                  | 10    | 0        | 0         | 0.0803 | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| 1,3-Dichloropropane       | A            | ug/L         | 263.47539  | 10.5390156    |                  | 10    | 0        | 0         | 0.0791 | 0.5    | 500    | 105% | 70  | 130  | 0%   |   |
| 1,4-Dichlorobenzene       | A            | ug/L         | 254.91697  | 10.1966788    |                  | 10    | 0        | 0         | 0.0858 | 0.5    | 500    | 102% | 70  | 130  | 0%   |   |
| 2,2-Dichloropropane       | A            | ug/L         | 253.03965  | 10.121586     |                  | 10    | 0        | 0         | 0.186  | 0.5    | 500    | 101% | 70  | 130  | 0%   |   |
| 2-Chlorotoluene           | A            | ug/L         | 267.26165  | 10.690466     |                  | 10    | 0        | 0         | 0.0876 | 0.5    | 500    | 107% | 70  | 130  | 0%   |   |
| 4-Chlorotoluene           | A            | ug/L         | 267.44092  | 10.6976368    |                  | 10    | 0        | 0         | 0.0728 | 0.5    | 500    | 107% | 70  | 130  | 0%   |   |
| Benzene                   | A            | ug/L         | 257.54165  | 10.301666     |                  | 10    | 0        | 0         | 0.0914 | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| Bromobenzene              | A            | ug/L         | 263.29438  | 10.5317752    |                  | 10    | 0        | 0         | 0.0831 | 0.5    | 500    | 105% | 70  | 130  | 0%   |   |
| Bromochloromethane        | A            | ug/L         | 247.05862  | 9.8823448     |                  | 10    | 0        | 0         | 0.141  | 0.5    | 500    | 99%  | 70  | 130  | 0%   |   |
| Bromodichloromethane      | A            | ug/L         | 257.22856  | 10.2891424    |                  | 10    | 0        | 0         | 0.12   | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| Bromoform                 | A            | ug/L         | 257.5099   | 10.300396     |                  | 10    | 0        | 0         | 0.119  | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| Bromomethane              | A            | ug/L         | 251.76065  | 10.070426     |                  | 10    | 0        | 0         | 0.253  | 0.5    | 500    | 101% | 70  | 130  | 0%   |   |
| Carbon tetrachloride      | A            | ug/L         | 260.87744  | 10.4350976    |                  | 10    | 0        | 0         | 0.143  | 0.5    | 500    | 104% | 70  | 130  | 0%   |   |
| Chlorobenzene             | A            | ug/L         | 258.25445  | 10.330178     |                  | 10    | 0        | 0         | 0.0914 | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| Chlorodibromomethane      | A            | ug/L         | 258.35353  | 10.3341412    |                  | 10    | 0        | 0         | 0.0841 | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |

| Seq No                         | Lab ID       | Test Code    | Sample Typ | File ID       | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|--------------------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970906                       | ICAL010422_6 | VOC-8260-W-Q | CAL6       | DA5975C\VG010 | 1/4/2022 6:45:10 | 1     | R372940  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                        | T            | Units        | RAW        | Final         | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| Chloroethane                   | A            | ug/L         | 231.74321  | 9.2697284     |                  | 10    | 0        | 0         | 0.169  | 0.5    | 500    | 93%  | 70  | 130  | 0%   |   |
| Chloroform                     | A            | ug/L         | 248.08043  | 9.9232172     |                  | 10    | 0        | 0         | 0.0789 | 0.5    | 500    | 99%  | 70  | 130  | 0%   |   |
| Chloromethane                  | A            | ug/L         | 240.2183   | 9.608732      |                  | 10    | 0        | 0         | 0.162  | 0.5    | 500    | 96%  | 70  | 130  | 0%   |   |
| cis-1,2-Dichloroethene         | A            | ug/L         | 261.87064  | 10.4748256    |                  | 10    | 0        | 0         | 0.108  | 0.5    | 500    | 105% | 70  | 130  | 0%   |   |
| cis-1,3-Dichloropropene        | A            | ug/L         | 265.28626  | 10.6114504    |                  | 10    | 0        | 0         | 0.073  | 0.5    | 500    | 106% | 70  | 130  | 0%   |   |
| Dibromomethane                 | A            | ug/L         | 252.27336  | 10.0909344    |                  | 10    | 0        | 0         | 0.147  | 0.5    | 500    | 101% | 70  | 130  | 0%   |   |
| Dichlorodifluoromethane        | A            | ug/L         | 252.15586  | 10.0862344    |                  | 10    | 0        | 0         | 0.175  | 0.5    | 500    | 101% | 70  | 130  | 0%   |   |
| Ethylbenzene                   | A            | ug/L         | 266.81931  | 10.6727724    |                  | 10    | 0        | 0         | 0.0836 | 0.5    | 500    | 107% | 70  | 130  | 0%   |   |
| m+p-Xylenes                    | A            | ug/L         | 543.42617  | 21.7370468    |                  | 20    | 0        | 0         | 0.15   | 0.5    | 1000   | 109% | 70  | 130  | 0%   |   |
| Methyl ethyl ketone            | A            | ug/L         | 2688.24739 | 107.529896    |                  | 100   | 0        | 0         | 1.77   | 10     | 5000   | 108% | 70  | 130  | 0%   |   |
| Methyl tert-butyl ether (MTBE) | A            | ug/L         | 258.95351  | 10.3581404    |                  | 10    | 0        | 0         | 0.101  | 0.5    | 500    | 104% | 70  | 130  | 0%   |   |
| Methylene chloride             | A            | ug/L         | 235.46573  | 9.4186292     |                  | 10    | 0        | 0         | 0.338  | 0.5    | 500    | 94%  | 70  | 130  | 0%   |   |
| o-Xylene                       | A            | ug/L         | 270.46357  | 10.8185428    |                  | 10    | 0        | 0         | 0.0604 | 0.5    | 500    | 108% | 70  | 130  | 0%   |   |
| Styrene                        | A            | ug/L         | 278.0455   | 11.12182      |                  | 10    | 0        | 0         | 0.067  | 0.5    | 500    | 111% | 70  | 130  | 0%   |   |
| Tetrachloroethene              | A            | ug/L         | 259.74185  | 10.389674     |                  | 10    | 0        | 0         | 0.0671 | 0.5    | 500    | 104% | 70  | 130  | 0%   |   |
| Toluene                        | A            | ug/L         | 263.13299  | 10.5253196    |                  | 10    | 0        | 0         | 0.0679 | 0.5    | 500    | 105% | 70  | 130  | 0%   |   |
| trans-1,2-Dichloroethene       | A            | ug/L         | 254.6608   | 10.186432     |                  | 10    | 0        | 0         | 0.125  | 0.5    | 500    | 102% | 70  | 130  | 0%   |   |
| trans-1,3-Dichloropropene      | A            | ug/L         | 263.80268  | 10.5521072    |                  | 10    | 0        | 0         | 0.0846 | 0.5    | 500    | 106% | 70  | 130  | 0%   |   |
| Trichloroethene                | A            | ug/L         | 262.29307  | 10.4917228    |                  | 10    | 0        | 0         | 0.0993 | 0.5    | 500    | 105% | 70  | 130  | 0%   |   |
| Trichlorofluoromethane         | A            | ug/L         | 259.05024  | 10.3620096    |                  | 10    | 0        | 0         | 0.134  | 0.5    | 500    | 104% | 70  | 130  | 0%   |   |
| Vinyl chloride                 | A            | ug/L         | 248.65325  | 9.94613       |                  | 10    | 0        | 0         | 0.153  | 0.5    | 500    | 99%  | 70  | 130  | 0%   |   |
| 1,4-Dichlorobenzene-d4         | I            | ug/L         | 250        | 10            |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 70  | 130  | 0%   |   |
| Chlorobenzene-d5               | I            | ug/L         | 250        | 10            |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 70  | 130  | 0%   |   |
| Fluorobenzene                  | I            | ug/L         | 250        | 10            |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 70  | 130  | 0%   |   |
| Xylenes, Total                 | M            | ug/L         | 813.88974  | 32.5555896    |                  | 30    | 0        | 0         | 0.0604 | 0.5    | 1500   | 109% | 70  | 130  | 0%   |   |
| 1,2-Dichloroethane-d4          | S            | ug/L         | 258.23239  | 10.3292956    |                  | 10    | 0        | 0         | 0.229  | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| Dibromofluoromethane           | S            | ug/L         | 259.02233  | 10.3608932    |                  | 10    | 0        | 0         | 0.129  | 0.5    | 500    | 104% | 70  | 130  | 0%   |   |
| p-Bromofluorobenzene           | S            | ug/L         | 267.31855  | 10.692742     |                  | 10    | 0        | 0         | 0.149  | 0.5    | 500    | 107% | 70  | 130  | 0%   |   |
| Toluene-d8                     | S            | ug/L         | 270.0265   | 10.80106      |                  | 10    | 0        | 0         | 0.23   | 0.5    | 500    | 108% | 70  | 130  | 0%   |   |

| Seq No   | Lab ID       | Test Code    | Sample Typ | File ID       | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|----------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970907 | ICAL010422_7 | VOC-8260-W-Q | CAL7       | DA5975C\VG010 | 1/4/2022 7:39:45 | 1     | R372940  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte  | T            | Units        | RAW        | Final         | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |

| Seq No                    | Lab ID       | Test Code    | Sample Typ | File ID       | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|---------------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970907                  | ICAL010422_7 | VOC-8260-W-Q | CAL7       | DA5975C\VG010 | 1/4/2022 7:39:45 | 1     | R372940  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                   | T            | Units        | RAW        | Final         | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A            | ug/L         | 392.18595  | 15.687438     |                  | 15    | 0        | 0         | 0.101  | 0.5    | 500    | 105% | 70  | 130  | 0%   |   |
| 1,1,1-Trichloroethane     | A            | ug/L         | 386.6625   | 15.4665       |                  | 15    | 0        | 0         | 0.131  | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| 1,1,2,2-Tetrachloroethane | A            | ug/L         | 367.42759  | 14.6971036    |                  | 15    | 0        | 0         | 0.0872 | 0.5    | 500    | 98%  | 70  | 130  | 0%   |   |
| 1,1,2-Trichloroethane     | A            | ug/L         | 373.25341  | 14.9301364    |                  | 15    | 0        | 0         | 0.108  | 0.5    | 500    | 100% | 70  | 130  | 0%   |   |
| 1,1-Dichloroethane        | A            | ug/L         | 380.44366  | 15.2177464    |                  | 15    | 0        | 0         | 0.135  | 0.5    | 500    | 101% | 70  | 130  | 0%   |   |
| 1,1-Dichloroethene        | A            | ug/L         | 380.37253  | 15.2149012    |                  | 15    | 0        | 0         | 0.141  | 0.5    | 500    | 101% | 70  | 130  | 0%   |   |
| 1,1-Dichloropropene       | A            | ug/L         | 397.13223  | 15.8852892    |                  | 15    | 0        | 0         | 0.083  | 0.5    | 500    | 106% | 70  | 130  | 0%   |   |
| 1,2,3-Trichloropropane    | A            | ug/L         | 363.67316  | 14.5469264    |                  | 15    | 0        | 0         | 0.235  | 0.5    | 500    | 97%  | 70  | 130  | 0%   |   |
| 1,2-Dibromoethane         | A            | ug/L         | 377.7698   | 15.110792     |                  | 15    | 0        | 0         | 0.0916 | 0.5    | 500    | 101% | 70  | 130  | 0%   |   |
| 1,2-Dichlorobenzene       | A            | ug/L         | 375.32826  | 15.0131304    |                  | 15    | 0        | 0         | 0.0746 | 0.5    | 500    | 100% | 70  | 130  | 0%   |   |
| 1,2-Dichloroethane        | A            | ug/L         | 366.9787   | 14.679148     |                  | 15    | 0        | 0         | 0.116  | 0.5    | 500    | 98%  | 70  | 130  | 0%   |   |
| 1,2-Dichloropropane       | A            | ug/L         | 388.85021  | 15.5540084    |                  | 15    | 0        | 0         | 0.0847 | 0.5    | 500    | 104% | 70  | 130  | 0%   |   |
| 1,3-Dichlorobenzene       | A            | ug/L         | 383.62247  | 15.3448988    |                  | 15    | 0        | 0         | 0.0803 | 0.5    | 500    | 102% | 70  | 130  | 0%   |   |
| 1,3-Dichloropropane       | A            | ug/L         | 389.34421  | 15.5737684    |                  | 15    | 0        | 0         | 0.0791 | 0.5    | 500    | 104% | 70  | 130  | 0%   |   |
| 1,4-Dichlorobenzene       | A            | ug/L         | 371.39689  | 14.8558756    |                  | 15    | 0        | 0         | 0.0858 | 0.5    | 500    | 99%  | 70  | 130  | 0%   |   |
| 2,2-Dichloropropane       | A            | ug/L         | 369.84356  | 14.7937424    |                  | 15    | 0        | 0         | 0.186  | 0.5    | 500    | 99%  | 70  | 130  | 0%   |   |
| 2-Chlorotoluene           | A            | ug/L         | 391.82688  | 15.6730752    |                  | 15    | 0        | 0         | 0.0876 | 0.5    | 500    | 104% | 70  | 130  | 0%   |   |
| 4-Chlorotoluene           | A            | ug/L         | 396.27563  | 15.8510252    |                  | 15    | 0        | 0         | 0.0728 | 0.5    | 500    | 106% | 70  | 130  | 0%   |   |
| Benzene                   | A            | ug/L         | 385.85261  | 15.4341044    |                  | 15    | 0        | 0         | 0.0914 | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| Bromobenzene              | A            | ug/L         | 386.44198  | 15.4576792    |                  | 15    | 0        | 0         | 0.0831 | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| Bromochloromethane        | A            | ug/L         | 371.80037  | 14.8720148    |                  | 15    | 0        | 0         | 0.141  | 0.5    | 500    | 99%  | 70  | 130  | 0%   |   |
| Bromodichloromethane      | A            | ug/L         | 386.19404  | 15.4477616    |                  | 15    | 0        | 0         | 0.12   | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| Bromoform                 | A            | ug/L         | 378.22002  | 15.1288008    |                  | 15    | 0        | 0         | 0.119  | 0.5    | 500    | 101% | 70  | 130  | 0%   |   |
| Bromomethane              | A            | ug/L         | 385.12594  | 15.4050376    |                  | 15    | 0        | 0         | 0.253  | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| Carbon tetrachloride      | A            | ug/L         | 386.9014   | 15.476056     |                  | 15    | 0        | 0         | 0.143  | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| Chlorobenzene             | A            | ug/L         | 386.94547  | 15.4778188    |                  | 15    | 0        | 0         | 0.0914 | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| Chlorodibromomethane      | A            | ug/L         | 387.68121  | 15.5072484    |                  | 15    | 0        | 0         | 0.0841 | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| Chloroethane              | A            | ug/L         | 364.45728  | 14.5782912    |                  | 15    | 0        | 0         | 0.169  | 0.5    | 500    | 97%  | 70  | 130  | 0%   |   |
| Chloroform                | A            | ug/L         | 366.93889  | 14.6775556    |                  | 15    | 0        | 0         | 0.0789 | 0.5    | 500    | 98%  | 70  | 130  | 0%   |   |
| Chloromethane             | A            | ug/L         | 352.08363  | 14.0833452    |                  | 15    | 0        | 0         | 0.162  | 0.5    | 500    | 94%  | 70  | 130  | 0%   |   |
| cis-1,2-Dichloroethene    | A            | ug/L         | 386.72365  | 15.468946     |                  | 15    | 0        | 0         | 0.108  | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| cis-1,3-Dichloropropene   | A            | ug/L         | 400.79296  | 16.0317184    |                  | 15    | 0        | 0         | 0.073  | 0.5    | 500    | 107% | 70  | 130  | 0%   |   |
| Dibromomethane            | A            | ug/L         | 380.65469  | 15.2261876    |                  | 15    | 0        | 0         | 0.147  | 0.5    | 500    | 102% | 70  | 130  | 0%   |   |
| Dichlorodifluoromethane   | A            | ug/L         | 373.94485  | 14.957794     |                  | 15    | 0        | 0         | 0.175  | 0.5    | 500    | 100% | 70  | 130  | 0%   |   |
| Ethylbenzene              | A            | ug/L         | 404.7587   | 16.190348     |                  | 15    | 0        | 0         | 0.0836 | 0.5    | 500    | 108% | 70  | 130  | 0%   |   |

| Seq No                         | Lab ID       | Test Code    | Sample Typ | File ID       | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|--------------------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970907                       | ICAL010422_7 | VOC-8260-W-Q | CAL7       | DA5975C\VG010 | 1/4/2022 7:39:45 | 1     | R372940  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                        | T            | Units        | RAW        | Final         | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| m+p-Xylenes                    | A            | ug/L         | 812.85557  | 32.5142228    |                  | 30    | 0        | 0         | 0.15   | 0.5    | 1000   | 108% | 70  | 130  | 0%   |   |
| Methyl ethyl ketone            | A            | ug/L         | 3961.341   | 158.45364     |                  | 150   | 0        | 0         | 1.77   | 10     | 5000   | 106% | 70  | 130  | 0%   |   |
| Methyl tert-butyl ether (MTBE) | A            | ug/L         | 391.17667  | 15.6470668    |                  | 15    | 0        | 0         | 0.101  | 0.5    | 500    | 104% | 70  | 130  | 0%   |   |
| Methylene chloride             | A            | ug/L         | 348.06663  | 13.9226652    |                  | 15    | 0        | 0         | 0.338  | 0.5    | 500    | 93%  | 70  | 130  | 0%   |   |
| o-Xylene                       | A            | ug/L         | 408.20432  | 16.3281728    |                  | 15    | 0        | 0         | 0.0604 | 0.5    | 500    | 109% | 70  | 130  | 0%   |   |
| Styrene                        | A            | ug/L         | 413.75947  | 16.5503788    |                  | 15    | 0        | 0         | 0.067  | 0.5    | 500    | 110% | 70  | 130  | 0%   |   |
| Tetrachloroethene              | A            | ug/L         | 382.87963  | 15.3151852    |                  | 15    | 0        | 0         | 0.0671 | 0.5    | 500    | 102% | 70  | 130  | 0%   |   |
| Toluene                        | A            | ug/L         | 397.01061  | 15.8804244    |                  | 15    | 0        | 0         | 0.0679 | 0.5    | 500    | 106% | 70  | 130  | 0%   |   |
| trans-1,2-Dichloroethene       | A            | ug/L         | 376.13673  | 15.0454692    |                  | 15    | 0        | 0         | 0.125  | 0.5    | 500    | 100% | 70  | 130  | 0%   |   |
| trans-1,3-Dichloropropene      | A            | ug/L         | 402.10977  | 16.0843908    |                  | 15    | 0        | 0         | 0.0846 | 0.5    | 500    | 107% | 70  | 130  | 0%   |   |
| Trichloroethene                | A            | ug/L         | 394.48959  | 15.7795836    |                  | 15    | 0        | 0         | 0.0993 | 0.5    | 500    | 105% | 70  | 130  | 0%   |   |
| Trichlorofluoromethane         | A            | ug/L         | 371.42899  | 14.8571596    |                  | 15    | 0        | 0         | 0.134  | 0.5    | 500    | 99%  | 70  | 130  | 0%   |   |
| Vinyl chloride                 | A            | ug/L         | 372.35639  | 14.8942556    |                  | 15    | 0        | 0         | 0.153  | 0.5    | 500    | 99%  | 70  | 130  | 0%   |   |
| 1,4-Dichlorobenzene-d4         | I            | ug/L         | 250        | 10            |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 70  | 130  | 0%   |   |
| Chlorobenzene-d5               | I            | ug/L         | 250        | 10            |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 70  | 130  | 0%   |   |
| Fluorobenzene                  | I            | ug/L         | 250        | 10            |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 70  | 130  | 0%   |   |
| Xylenes, Total                 | M            | ug/L         | 1221.05989 | 48.8423956    |                  | 45    | 0        | 0         | 0.0604 | 0.5    | 1500   | 109% | 70  | 130  | 0%   |   |
| 1,2-Dichloroethane-d4          | S            | ug/L         | 378.33349  | 15.1333396    |                  | 15    | 0        | 0         | 0.229  | 0.5    | 500    | 101% | 70  | 130  | 0%   |   |
| Dibromofluoromethane           | S            | ug/L         | 384.7503   | 15.390012     |                  | 15    | 0        | 0         | 0.129  | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| p-Bromofluorobenzene           | S            | ug/L         | 394.65655  | 15.786262     |                  | 15    | 0        | 0         | 0.149  | 0.5    | 500    | 105% | 70  | 130  | 0%   |   |
| Toluene-d8                     | S            | ug/L         | 405.5583   | 16.222332     |                  | 15    | 0        | 0         | 0.23   | 0.5    | 500    | 108% | 70  | 130  | 0%   |   |

| Seq No                    | Lab ID       | Test Code    | Sample Typ | File ID       | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|---------------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970908                  | ICAL010422_8 | VOC-8260-W-Q | CAL8       | DA5975C\VG010 | 1/4/2022 8:34:31 | 1     | R372940  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                   | T            | Units        | RAW        | Final         | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A            | ug/L         | 520.28551  | 20.8114204    |                  | 20    | 0        | 0         | 0.101  | 0.5    | 500    | 104% | 70  | 130  | 0%   |   |
| 1,1,1-Trichloroethane     | A            | ug/L         | 518.83124  | 20.7532496    |                  | 20    | 0        | 0         | 0.131  | 0.5    | 500    | 104% | 70  | 130  | 0%   |   |
| 1,1,2,2-Tetrachloroethane | A            | ug/L         | 491.66999  | 19.6667996    |                  | 20    | 0        | 0         | 0.0872 | 0.5    | 500    | 98%  | 70  | 130  | 0%   |   |
| 1,1,2-Trichloroethane     | A            | ug/L         | 505.18031  | 20.2072124    |                  | 20    | 0        | 0         | 0.108  | 0.5    | 500    | 101% | 70  | 130  | 0%   |   |
| 1,1-Dichloroethane        | A            | ug/L         | 515.3207   | 20.612828     |                  | 20    | 0        | 0         | 0.135  | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| 1,1-Dichloroethene        | A            | ug/L         | 515.06031  | 20.6024124    |                  | 20    | 0        | 0         | 0.141  | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| 1,1-Dichloropropene       | A            | ug/L         | 543.51208  | 21.7404832    |                  | 20    | 0        | 0         | 0.083  | 0.5    | 500    | 109% | 70  | 130  | 0%   |   |
| 1,2,3-Trichloropropane    | A            | ug/L         | 491.52294  | 19.6609176    |                  | 20    | 0        | 0         | 0.235  | 0.5    | 500    | 98%  | 70  | 130  | 0%   |   |
| 1,2-Dibromoethane         | A            | ug/L         | 507.9234   | 20.316936     |                  | 20    | 0        | 0         | 0.0916 | 0.5    | 500    | 102% | 70  | 130  | 0%   |   |

| Seq No                         | Lab ID       | Test Code    | Sample Typ | File ID       | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|--------------------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970908                       | ICAL010422_8 | VOC-8260-W-Q | CAL8       | DA5975C\VG010 | 1/4/2022 8:34:31 | 1     | R372940  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                        | T            | Units        | RAW        | Final         | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| 1,2-Dichlorobenzene            | A            | ug/L         | 506.38707  | 20.2554828    |                  | 20    | 0        | 0         | 0.0746 | 0.5    | 500    | 101% | 70  | 130  | 0%   |   |
| 1,2-Dichloroethane             | A            | ug/L         | 497.36991  | 19.8947964    |                  | 20    | 0        | 0         | 0.116  | 0.5    | 500    | 99%  | 70  | 130  | 0%   |   |
| 1,2-Dichloropropane            | A            | ug/L         | 524.16945  | 20.966778     |                  | 20    | 0        | 0         | 0.0847 | 0.5    | 500    | 105% | 70  | 130  | 0%   |   |
| 1,3-Dichlorobenzene            | A            | ug/L         | 511.55042  | 20.4620168    |                  | 20    | 0        | 0         | 0.0803 | 0.5    | 500    | 102% | 70  | 130  | 0%   |   |
| 1,3-Dichloropropane            | A            | ug/L         | 511.24793  | 20.4499172    |                  | 20    | 0        | 0         | 0.0791 | 0.5    | 500    | 102% | 70  | 130  | 0%   |   |
| 1,4-Dichlorobenzene            | A            | ug/L         | 502.30007  | 20.0920028    |                  | 20    | 0        | 0         | 0.0858 | 0.5    | 500    | 100% | 70  | 130  | 0%   |   |
| 2,2-Dichloropropane            | A            | ug/L         | 499.04726  | 19.9618904    |                  | 20    | 0        | 0         | 0.186  | 0.5    | 500    | 100% | 70  | 130  | 0%   |   |
| 2-Chlorotoluene                | A            | ug/L         | 538.49638  | 21.5398552    |                  | 20    | 0        | 0         | 0.0876 | 0.5    | 500    | 108% | 70  | 130  | 0%   |   |
| 4-Chlorotoluene                | A            | ug/L         | 531.84706  | 21.2738824    |                  | 20    | 0        | 0         | 0.0728 | 0.5    | 500    | 106% | 70  | 130  | 0%   |   |
| Benzene                        | A            | ug/L         | 511.66576  | 20.4666304    |                  | 20    | 0        | 0         | 0.0914 | 0.5    | 500    | 102% | 70  | 130  | 0%   |   |
| Bromobenzene                   | A            | ug/L         | 516.0104   | 20.640416     |                  | 20    | 0        | 0         | 0.0831 | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| Bromochloromethane             | A            | ug/L         | 494.60544  | 19.7842176    |                  | 20    | 0        | 0         | 0.141  | 0.5    | 500    | 99%  | 70  | 130  | 0%   |   |
| Bromodichloromethane           | A            | ug/L         | 518.37176  | 20.7348704    |                  | 20    | 0        | 0         | 0.12   | 0.5    | 500    | 104% | 70  | 130  | 0%   |   |
| Bromoform                      | A            | ug/L         | 522.76605  | 20.910642     |                  | 20    | 0        | 0         | 0.119  | 0.5    | 500    | 105% | 70  | 130  | 0%   |   |
| Bromomethane                   | A            | ug/L         | 515.01414  | 20.6005656    |                  | 20    | 0        | 0         | 0.253  | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| Carbon tetrachloride           | A            | ug/L         | 521.26297  | 20.8505188    |                  | 20    | 0        | 0         | 0.143  | 0.5    | 500    | 104% | 70  | 130  | 0%   |   |
| Chlorobenzene                  | A            | ug/L         | 515.99575  | 20.63983      |                  | 20    | 0        | 0         | 0.0914 | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| Chlorodibromomethane           | A            | ug/L         | 520.43607  | 20.8174428    |                  | 20    | 0        | 0         | 0.0841 | 0.5    | 500    | 104% | 70  | 130  | 0%   |   |
| Chloroethane                   | A            | ug/L         | 481.51432  | 19.2605728    |                  | 20    | 0        | 0         | 0.169  | 0.5    | 500    | 96%  | 70  | 130  | 0%   |   |
| Chloroform                     | A            | ug/L         | 489.12212  | 19.5648848    |                  | 20    | 0        | 0         | 0.0789 | 0.5    | 500    | 98%  | 70  | 130  | 0%   |   |
| Chloromethane                  | A            | ug/L         | 480.17469  | 19.2069876    |                  | 20    | 0        | 0         | 0.162  | 0.5    | 500    | 96%  | 70  | 130  | 0%   |   |
| cis-1,2-Dichloroethene         | A            | ug/L         | 516.05445  | 20.642178     |                  | 20    | 0        | 0         | 0.108  | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| cis-1,3-Dichloropropene        | A            | ug/L         | 538.90085  | 21.556034     |                  | 20    | 0        | 0         | 0.073  | 0.5    | 500    | 108% | 70  | 130  | 0%   |   |
| Dibromomethane                 | A            | ug/L         | 500.74556  | 20.0298224    |                  | 20    | 0        | 0         | 0.147  | 0.5    | 500    | 100% | 70  | 130  | 0%   |   |
| Dichlorodifluoromethane        | A            | ug/L         | 494.74738  | 19.7898952    |                  | 20    | 0        | 0         | 0.175  | 0.5    | 500    | 99%  | 70  | 130  | 0%   |   |
| Ethylbenzene                   | A            | ug/L         | 544.68805  | 21.787522     |                  | 20    | 0        | 0         | 0.0836 | 0.5    | 500    | 109% | 70  | 130  | 0%   |   |
| m+p-Xylenes                    | A            | ug/L         | 1087.40818 | 43.4963272    |                  | 40    | 0        | 0         | 0.15   | 0.5    | 1000   | 109% | 70  | 130  | 0%   |   |
| Methyl ethyl ketone            | A            | ug/L         | 5327.12526 | 213.085010    |                  | 200   | 0        | 0         | 1.77   | 10     | 5000   | 107% | 70  | 130  | 0%   |   |
| Methyl tert-butyl ether (MTBE) | A            | ug/L         | 522.81865  | 20.912746     |                  | 20    | 0        | 0         | 0.101  | 0.5    | 500    | 105% | 70  | 130  | 0%   |   |
| Methylene chloride             | A            | ug/L         | 466.99932  | 18.6799728    |                  | 20    | 0        | 0         | 0.338  | 0.5    | 500    | 93%  | 70  | 130  | 0%   |   |
| o-Xylene                       | A            | ug/L         | 547.47638  | 21.8990552    |                  | 20    | 0        | 0         | 0.0604 | 0.5    | 500    | 109% | 70  | 130  | 0%   |   |
| Styrene                        | A            | ug/L         | 555.79455  | 22.231782     |                  | 20    | 0        | 0         | 0.067  | 0.5    | 500    | 111% | 70  | 130  | 0%   |   |
| Tetrachloroethene              | A            | ug/L         | 514.92548  | 20.5970192    |                  | 20    | 0        | 0         | 0.0671 | 0.5    | 500    | 103% | 70  | 130  | 0%   |   |
| Toluene                        | A            | ug/L         | 536.51007  | 21.4604028    |                  | 20    | 0        | 0         | 0.0679 | 0.5    | 500    | 107% | 70  | 130  | 0%   |   |
| trans-1,2-Dichloroethene       | A            | ug/L         | 510.00974  | 20.4003896    |                  | 20    | 0        | 0         | 0.125  | 0.5    | 500    | 102% | 70  | 130  | 0%   |   |

| Seq No                    | Lab ID       | Test Code    | Sample Typ | File ID       | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|---------------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970908                  | ICAL010422_8 | VOC-8260-W-Q | CAL8       | DA5975C\VG010 | 1/4/2022 8:34:31 | 1     | R372940  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                   | T            | Units        | RAW        | Final         | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| trans-1,3-Dichloropropene | A            | ug/L         | 533.75507  | 21.3502028    |                  | 20    | 0        | 0         | 0.0846 | 0.5    | 500    | 107% | 70  | 130  | 0%   |   |
| Trichloroethene           | A            | ug/L         | 534.40073  | 21.3760292    |                  | 20    | 0        | 0         | 0.0993 | 0.5    | 500    | 107% | 70  | 130  | 0%   |   |
| Trichlorofluoromethane    | A            | ug/L         | 489.6475   | 19.5859       |                  | 20    | 0        | 0         | 0.134  | 0.5    | 500    | 98%  | 70  | 130  | 0%   |   |
| Vinyl chloride            | A            | ug/L         | 498.3563   | 19.934252     |                  | 20    | 0        | 0         | 0.153  | 0.5    | 500    | 100% | 70  | 130  | 0%   |   |
| 1,4-Dichlorobenzene-d4    | I            | ug/L         | 250        | 10            |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 70  | 130  | 0%   |   |
| Chlorobenzene-d5          | I            | ug/L         | 250        | 10            |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 70  | 130  | 0%   |   |
| Fluorobenzene             | I            | ug/L         | 250        | 10            |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 70  | 130  | 0%   |   |
| Xylenes, Total            | M            | ug/L         | 1634.88456 | 65.3953824    |                  | 60    | 0        | 0         | 0.0604 | 0.5    | 1500   | 109% | 70  | 130  | 0%   |   |
| 1,2-Dichloroethane-d4     | S            | ug/L         | 510.30803  | 20.4123212    |                  | 20    | 0        | 0         | 0.229  | 0.5    | 500    | 102% | 70  | 130  | 0%   |   |
| Dibromofluoromethane      | S            | ug/L         | 510.39915  | 20.415966     |                  | 20    | 0        | 0         | 0.129  | 0.5    | 500    | 102% | 70  | 130  | 0%   |   |
| p-Bromofluorobenzene      | S            | ug/L         | 541.3964   | 21.655856     |                  | 20    | 0        | 0         | 0.149  | 0.5    | 500    | 108% | 70  | 130  | 0%   |   |
| Toluene-d8                | S            | ug/L         | 544.21357  | 21.7685428    |                  | 20    | 0        | 0         | 0.23   | 0.5    | 500    | 109% | 70  | 130  | 0%   |   |

| Seq No                    | Lab ID    | Test Code    | Sample Typ | File ID       | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|---------------------------|-----------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970909                  | ICV010422 | VOC-8260-W-Q | ICV        | DA5975C\VG010 | 1/4/2022 9:29:14 | 1     | R372940  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                   | T         | Units        | RAW        | Final         | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A         | ug/L         | 126.66575  | 5.06663       |                  | 5     | 0        | 0         | 0.101  | 0.5    | 500    | 101% | 80  | 120  | 0%   |   |
| 1,1,1-Trichloroethane     | A         | ug/L         | 128.25238  | 5.1300952     |                  | 5     | 0        | 0         | 0.131  | 0.5    | 500    | 103% | 80  | 120  | 0%   |   |
| 1,1,2,2-Tetrachloroethane | A         | ug/L         | 127.47217  | 5.0988868     |                  | 5     | 0        | 0         | 0.0872 | 0.5    | 500    | 102% | 80  | 120  | 0%   |   |
| 1,1,2-Trichloroethane     | A         | ug/L         | 123.03611  | 4.9214444     |                  | 5     | 0        | 0         | 0.108  | 0.5    | 500    | 98%  | 80  | 120  | 0%   |   |
| 1,1-Dichloroethane        | A         | ug/L         | 135.803    | 5.43212       |                  | 5     | 0        | 0         | 0.135  | 0.5    | 500    | 109% | 80  | 120  | 0%   |   |
| 1,1-Dichloroethene        | A         | ug/L         | 134.45663  | 5.3782652     |                  | 5     | 0        | 0         | 0.141  | 0.5    | 500    | 108% | 80  | 120  | 0%   |   |
| 1,1-Dichloropropene       | A         | ug/L         | 124.18526  | 4.9674104     |                  | 5     | 0        | 0         | 0.083  | 0.5    | 500    | 99%  | 80  | 120  | 0%   |   |
| 1,2,3-Trichloropropane    | A         | ug/L         | 122.95232  | 4.9180928     |                  | 5     | 0        | 0         | 0.235  | 0.5    | 500    | 98%  | 80  | 120  | 0%   |   |
| 1,2-Dibromoethane         | A         | ug/L         | 124.27642  | 4.9710568     |                  | 5     | 0        | 0         | 0.0916 | 0.5    | 500    | 99%  | 80  | 120  | 0%   |   |
| 1,2-Dichlorobenzene       | A         | ug/L         | 128.71039  | 5.1484156     |                  | 5     | 0        | 0         | 0.0746 | 0.5    | 500    | 103% | 80  | 120  | 0%   |   |
| 1,2-Dichloroethane        | A         | ug/L         | 120.79914  | 4.8319656     |                  | 5     | 0        | 0         | 0.116  | 0.5    | 500    | 97%  | 80  | 120  | 0%   |   |
| 1,2-Dichloropropane       | A         | ug/L         | 125.66265  | 5.026506      |                  | 5     | 0        | 0         | 0.0847 | 0.5    | 500    | 101% | 80  | 120  | 0%   |   |
| 1,3-Dichlorobenzene       | A         | ug/L         | 135.11854  | 5.4047416     |                  | 5     | 0        | 0         | 0.0803 | 0.5    | 500    | 108% | 80  | 120  | 0%   |   |
| 1,3-Dichloropropane       | A         | ug/L         | 121.84417  | 4.8737668     |                  | 5     | 0        | 0         | 0.0791 | 0.5    | 500    | 97%  | 80  | 120  | 0%   |   |
| 1,4-Dichlorobenzene       | A         | ug/L         | 129.88123  | 5.1952492     |                  | 5     | 0        | 0         | 0.0858 | 0.5    | 500    | 104% | 80  | 120  | 0%   |   |
| 2,2-Dichloropropane       | A         | ug/L         | 131.40305  | 5.256122      |                  | 5     | 0        | 0         | 0.186  | 0.5    | 500    | 105% | 80  | 120  | 0%   |   |
| 2-Chlorotoluene           | A         | ug/L         | 131.29475  | 5.25179       |                  | 5     | 0        | 0         | 0.0876 | 0.5    | 500    | 105% | 80  | 120  | 0%   |   |
| 4-Chlorotoluene           | A         | ug/L         | 137.07902  | 5.4831608     |                  | 5     | 0        | 0         | 0.0728 | 0.5    | 500    | 110% | 80  | 120  | 0%   |   |



| Seq No                         | Lab ID    | Test Code    | Sample Typ | File ID       | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|--------------------------------|-----------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970909                       | ICV010422 | VOC-8260-W-Q | ICV        | DA5975C\VG010 | 1/4/2022 9:29:14 | 1     | R372940  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                        | T         | Units        | RAW        | Final         | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| Benzene                        | A         | ug/L         | 131.31393  | 5.2525572     |                  | 5     | 0        | 0         | 0.0914 | 0.5    | 500    | 105% | 80  | 120  | 0%   |   |
| Bromobenzene                   | A         | ug/L         | 131.67879  | 5.2671516     |                  | 5     | 0        | 0         | 0.0831 | 0.5    | 500    | 105% | 80  | 120  | 0%   |   |
| Bromochloromethane             | A         | ug/L         | 123.60094  | 4.9440376     |                  | 5     | 0        | 0         | 0.141  | 0.5    | 500    | 99%  | 80  | 120  | 0%   |   |
| Bromodichloromethane           | A         | ug/L         | 128.87588  | 5.1550352     |                  | 5     | 0        | 0         | 0.12   | 0.5    | 500    | 103% | 80  | 120  | 0%   |   |
| Bromoform                      | A         | ug/L         | 129.9644   | 5.198576      |                  | 5     | 0        | 0         | 0.119  | 0.5    | 500    | 104% | 80  | 120  | 0%   |   |
| Bromomethane                   | A         | ug/L         | 116.91567  | 4.6766268     |                  | 5     | 0        | 0         | 0.253  | 0.5    | 500    | 94%  | 80  | 120  | 0%   |   |
| Carbon tetrachloride           | A         | ug/L         | 128.79275  | 5.15171       |                  | 5     | 0        | 0         | 0.143  | 0.5    | 500    | 103% | 80  | 120  | 0%   |   |
| Chlorobenzene                  | A         | ug/L         | 131.63517  | 5.2654068     |                  | 5     | 0        | 0         | 0.0914 | 0.5    | 500    | 105% | 80  | 120  | 0%   |   |
| Chlorodibromomethane           | A         | ug/L         | 125.11031  | 5.0044124     |                  | 5     | 0        | 0         | 0.0841 | 0.5    | 500    | 100% | 80  | 120  | 0%   |   |
| Chloroethane                   | A         | ug/L         | 115.59324  | 4.6237296     |                  | 5     | 0        | 0         | 0.169  | 0.5    | 500    | 92%  | 80  | 120  | 0%   |   |
| Chloroform                     | A         | ug/L         | 120.42358  | 4.8169432     |                  | 5     | 0        | 0         | 0.0789 | 0.5    | 500    | 96%  | 80  | 120  | 0%   |   |
| Chloromethane                  | A         | ug/L         | 108.77392  | 4.3509568     |                  | 5     | 0        | 0         | 0.162  | 0.5    | 500    | 87%  | 80  | 120  | 0%   |   |
| cis-1,2-Dichloroethene         | A         | ug/L         | 130.12309  | 5.2049236     |                  | 5     | 0        | 0         | 0.108  | 0.5    | 500    | 104% | 80  | 120  | 0%   |   |
| cis-1,3-Dichloropropene        | A         | ug/L         | 121.55615  | 4.862246      |                  | 5     | 0        | 0         | 0.073  | 0.5    | 500    | 97%  | 80  | 120  | 0%   |   |
| Dibromomethane                 | A         | ug/L         | 125.30472  | 5.0121888     |                  | 5     | 0        | 0         | 0.147  | 0.5    | 500    | 100% | 80  | 120  | 0%   |   |
| Dichlorodifluoromethane        | A         | ug/L         | 111.37489  | 4.4549956     |                  | 5     | 0        | 0         | 0.175  | 0.5    | 500    | 89%  | 80  | 120  | 0%   |   |
| Ethylbenzene                   | A         | ug/L         | 131.91134  | 5.2764536     |                  | 5     | 0        | 0         | 0.0836 | 0.5    | 500    | 106% | 80  | 120  | 0%   |   |
| m+p-Xylenes                    | A         | ug/L         | 262.75886  | 10.5103544    |                  | 10    | 0        | 0         | 0.15   | 0.5    | 1000   | 105% | 80  | 120  | 0%   |   |
| Methyl ethyl ketone            | A         | ug/L         | 1198.44392 | 47.9377568    |                  | 50    | 0        | 0         | 1.77   | 10     | 5000   | 96%  | 80  | 120  | 0%   |   |
| Methyl tert-butyl ether (MTBE) | A         | ug/L         | 134.72237  | 5.3888948     |                  | 5     | 0        | 0         | 0.101  | 0.5    | 500    | 108% | 80  | 120  | 0%   |   |
| Methylene chloride             | A         | ug/L         | 121.52968  | 4.8611872     |                  | 5     | 0        | 0         | 0.338  | 0.5    | 500    | 97%  | 80  | 120  | 0%   |   |
| o-Xylene                       | A         | ug/L         | 132.22141  | 5.2888564     |                  | 5     | 0        | 0         | 0.0604 | 0.5    | 500    | 106% | 80  | 120  | 0%   |   |
| Styrene                        | A         | ug/L         | 137.49736  | 5.4998944     |                  | 5     | 0        | 0         | 0.067  | 0.5    | 500    | 110% | 80  | 120  | 0%   |   |
| Tetrachloroethene              | A         | ug/L         | 126.01413  | 5.0405652     |                  | 5     | 0        | 0         | 0.0671 | 0.5    | 500    | 101% | 80  | 120  | 0%   |   |
| Toluene                        | A         | ug/L         | 132.0244   | 5.280976      |                  | 5     | 0        | 0         | 0.0679 | 0.5    | 500    | 106% | 80  | 120  | 0%   |   |
| trans-1,2-Dichloroethene       | A         | ug/L         | 134.70283  | 5.3881132     |                  | 5     | 0        | 0         | 0.125  | 0.5    | 500    | 108% | 80  | 120  | 0%   |   |
| trans-1,3-Dichloropropene      | A         | ug/L         | 129.02156  | 5.1608624     |                  | 5     | 0        | 0         | 0.0846 | 0.5    | 500    | 103% | 80  | 120  | 0%   |   |
| Trichloroethene                | A         | ug/L         | 131.10958  | 5.2443832     |                  | 5     | 0        | 0         | 0.0993 | 0.5    | 500    | 105% | 80  | 120  | 0%   |   |
| Trichlorofluoromethane         | A         | ug/L         | 121.7847   | 4.871388      |                  | 5     | 0        | 0         | 0.134  | 0.5    | 500    | 97%  | 80  | 120  | 0%   |   |
| Vinyl chloride                 | A         | ug/L         | 120.15175  | 4.80607       |                  | 5     | 0        | 0         | 0.153  | 0.5    | 500    | 96%  | 80  | 120  | 0%   |   |
| 1,4-Dichlorobenzene-d4         | I         | ug/L         | 250        | 10            |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 0   | 0    | 0%   |   |
| Chlorobenzene-d5               | I         | ug/L         | 250        | 10            |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 0   | 0    | 0%   |   |
| Fluorobenzene                  | I         | ug/L         | 250        | 10            |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 0   | 0    | 0%   |   |
| Xylenes, Total                 | M         | ug/L         | 394.98027  | 15.7992108    |                  | 15    | 0        | 0         | 0.0604 | 0.5    | 1500   | 105% | 80  | 120  | 0%   |   |
| 1,2-Dichloroethane-d4          | S         | ug/L         | 280.28858  | 11.2115432    |                  | 10    | 0        | 0         | 0.229  | 0.5    | 500    | 112% | 80  | 120  | 0%   |   |

| Seq No               | Lab ID    | Test Code    | Sample Typ | File ID       | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|----------------------|-----------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14970909             | ICV010422 | VOC-8260-W-Q | ICV        | DA5975C\VG010 | 1/4/2022 9:29:14 | 1     | R372940  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte              | T         | Units        | RAW        | Final         | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| Dibromofluoromethane | S         | ug/L         | 271.19937  | 10.8479748    |                  | 10    | 0        | 0         | 0.129  | 0.5    | 500    | 108% | 80  | 120  | 0%   |   |
| p-Bromofluorobenzene | S         | ug/L         | 269.89759  | 10.7959036    |                  | 10    | 0        | 0         | 0.149  | 0.5    | 500    | 108% | 80  | 120  | 0%   |   |
| Toluene-d8           | S         | ug/L         | 276.91062  | 11.0764248    |                  | 10    | 0        | 0         | 0.23   | 0.5    | 500    | 111% | 80  | 120  | 0%   |   |

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN01.D  
Sample Name : PRIMER  
Operator : MSC  
Date injected : 4 Jan 2022 9:44 am  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 1

---

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN02.D  
Sample Name : BFB010422\_  
Operator : MSC  
Date injected : 4 Jan 2022 10:11 am  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 2

---

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN03.D  
Sample Name : CCV010422\_  
Operator : MSC  
Date injected : 4 Jan 2022 10:56 am  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 3

---

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN04.D  
Sample Name : PRIMER  
Misc. Info. : Replaced purge trap  
Operator : MSC  
Date injected : 4 Jan 2022 12:17 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 4

---

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN05.D  
Sample Name : BFB010422\_

Operator : MSC  
Date injected : 4 Jan 2022 12:44 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 5

---

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN06.D  
Sample Name : CCV010422\_  
Operator : MSC  
Date injected : 4 Jan 2022 1:24 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 6

---

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN07.D  
Sample Name : BLK  
Operator : MSC  
Date injected : 4 Jan 2022 2:09 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.839  
End Time : 16.498  
Vial Number : 7

---

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN08.D  
Sample Name : BFB010422\_  
Operator : MSC  
Date injected : 4 Jan 2022 2:38 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 8

---

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN09.D  
Sample Name : MBLK010422\_  
Operator : MSC  
Date injected : 4 Jan 2022 3:05 pm  
Instrument : VOA5975C

Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 9

---

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN10.D  
Sample Name : ICAL010422\_1  
Operator : MSC  
Date injected : 4 Jan 2022 3:33 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 10

---

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN11.D  
Sample Name : ICAL010422\_2  
Operator : MSC  
Date injected : 4 Jan 2022 4:00 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 11

---

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN12.D  
Sample Name : ICAL010422\_3  
Operator : MSC  
Date injected : 4 Jan 2022 4:28 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 12

---

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN13.D  
Sample Name : ICAL010422\_4  
Operator : MSC  
Date injected : 4 Jan 2022 4:55 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840

End Time : 16.498  
Vial Number : 13

---

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN14.D  
Sample Name : BLK  
Operator : MSC  
Date injected : 4 Jan 2022 5:22 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 14

---

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN15.D  
Sample Name : ICAL010422\_5  
Operator : MSC  
Date injected : 4 Jan 2022 5:50 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 15

---

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN16.D  
Sample Name : BLK  
Operator : MSC  
Date injected : 4 Jan 2022 6:17 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 16

---

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN17.D  
Sample Name : ICAL010422\_6  
Operator : MSC  
Date injected : 4 Jan 2022 6:45 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 17

---

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN18.D  
Sample Name : BLK  
Operator : MSC  
Date injected : 4 Jan 2022 7:12 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 18

---

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN19.D  
Sample Name : ICAL010422\_7  
Operator : MSC  
Date injected : 4 Jan 2022 7:39 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 19

---

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN20.D  
Sample Name : BLK  
Operator : MSC  
Date injected : 4 Jan 2022 8:07 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.839  
End Time : 16.498  
Vial Number : 20

---

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN21.D  
Sample Name : ICAL010422\_8  
Operator : MSC  
Date injected : 4 Jan 2022 8:34 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 21

---

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN22.D  
Sample Name : BLK

Operator : MSC  
Date injected : 4 Jan 2022 9:01 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.839  
End Time : 16.498  
Vial Number : 22

---

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN23.D  
Sample Name : ICV010422  
Operator : MSC  
Date injected : 4 Jan 2022 9:29 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 23

---

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN24.D  
Sample Name : BLK  
Operator : MSC  
Date injected : 4 Jan 2022 9:56 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.839  
End Time : 16.498  
Vial Number : 24

---

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN25.D  
Sample Name : MDL010422\_Q1\_1  
Operator : MSC  
Date injected : 4 Jan 2022 10:23 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 25

---

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN26.D  
Sample Name : LOD010422\_Q1\_HalfCAL2  
Operator : MSC  
Date injected : 4 Jan 2022 10:51 pm  
Instrument : VOA5975C



Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.839  
End Time : 16.498  
Vial Number : 26

---

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN27.D  
Sample Name : MDL010422\_Q1\_2xCAL1  
Operator : MSC  
Date injected : 4 Jan 2022 11:18 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 27



---

Data file Name : C:\MSDCHEM\1\DATA\VG010422\04JAN28.D  
Sample Name : BLK  
Operator : MSC  
Date injected : 4 Jan 2022 11:45 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 28

---

# Tune Evaluation Report

Data Path: D:\Org\Data\VOA5975C\VG010422\04JAN08.D  
 Acq on: 1/4/2022 2:38:09 PM  
 Operator: MSC  
 Sample: BFB010422\_  
 Inst Name: VOA5975C  
 ALS Vial: 8  
 Method: \\MASSHUNTER\Org\Data\Methods\BFBapex.m

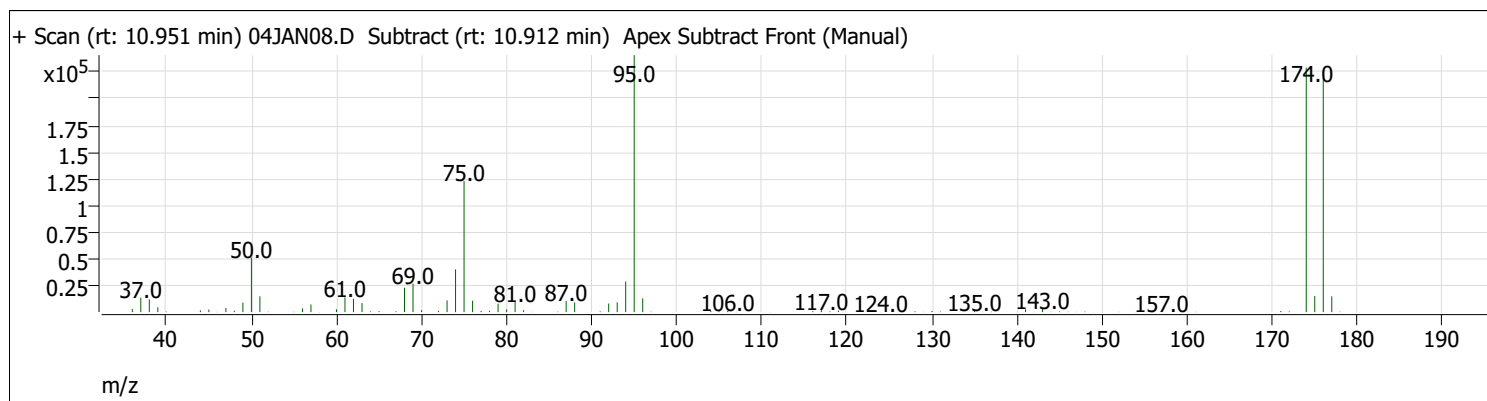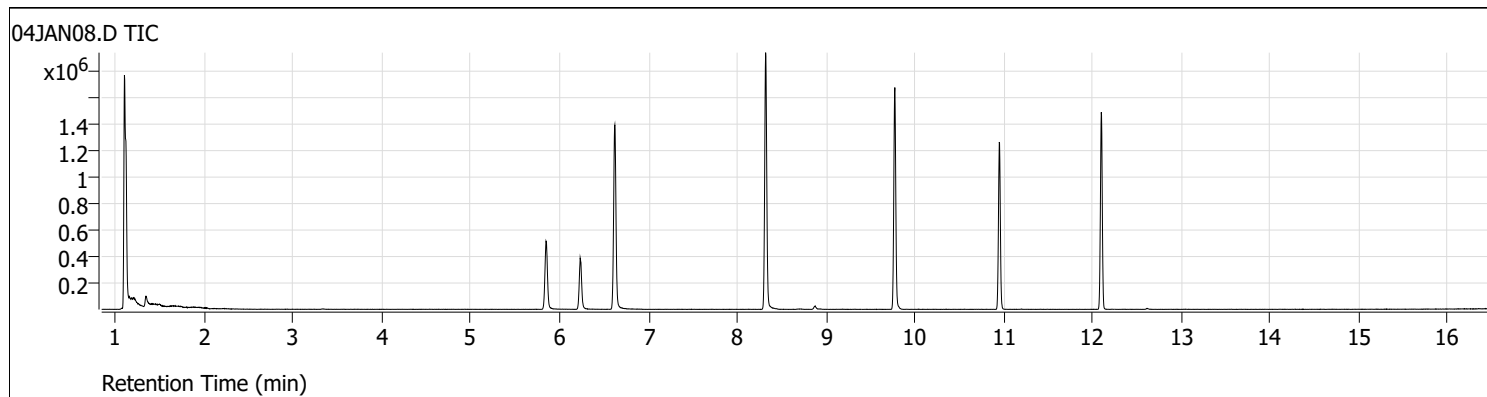

| Target Mass | Rel. To Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|-----------|
| 50          | 95           | 15           | 40           | 21.2      | 51080   | Pass      |
| 75          | 95           | 30           | 60           | 51.0      | 122824  | Pass      |
| 95          | 95           | 100          | 100          | 100.0     | 240768  | Pass      |
| 96          | 95           | 5            | 9            | 5.4       | 12961   | Pass      |
| 173         | 174          | 0            | 2            | 0.0       | 0       | Pass      |
| 174         | 95           | 50           | 100          | 95.2      | 229120  | Pass      |
| 175         | 174          | 5            | 9            | 6.6       | 15102   | Pass      |
| 176         | 174          | 95           | 101          | 95.7      | 219264  | Pass      |
| 177         | 176          | 5            | 9            | 6.7       | 14796   | Pass      |

# Quantitative Analysis Results Summary Report

|                     |                                                                     |                      |                |
|---------------------|---------------------------------------------------------------------|----------------------|----------------|
| Batch Path          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name         | BL2000\mchavez |
| Analysis Time       | 2/28/2022 1:57 PM                                                   | Reporter Name        | BL2000\mchavez |
| Report Time         | 2/28/2022 2:00:48 PM                                                | Batch State          | Processed      |
| Last Calib Update   | 1/9/2022 8:59 PM                                                    | Quant Report Version | 10.0           |
| Quant Batch Version | 10.0                                                                |                      |                |

## Sequence Table

| Data File | sample Name  | Sample Type  | Vial Position | Inj Vol | Level | Acq Method File |
|-----------|--------------|--------------|---------------|---------|-------|-----------------|
| 04JAN09.D | MBLK010422_  | Method Blank | 9             | 0       |       | 5975CACQF.M     |
| 04JAN10.D | ICAL010422_1 | Cal          | 10            | 0       | 1     | 5975CACQF.M     |
| 04JAN11.D | ICAL010422_2 | Cal          | 11            | 0       | 2     | 5975CACQF.M     |
| 04JAN12.D | ICAL010422_3 | Cal          | 12            | 0       | 3     | 5975CACQF.M     |
| 04JAN13.D | ICAL010422_4 | Cal          | 13            | 0       | 4     | 5975CACQF.M     |
| 04JAN15.D | ICAL010422_5 | Cal          | 15            | 0       | 5     | 5975CACQF.M     |
| 04JAN17.D | ICAL010422_6 | Cal          | 17            | 0       | 6     | 5975CACQF.M     |
| 04JAN19.D | ICAL010422_7 | Cal          | 19            | 0       | 7     | 5975CACQF.M     |
| 04JAN21.D | ICAL010422_8 | Cal          | 21            | 0       | 8     | 5975CACQF.M     |
| 04JAN23.D | ICV010422    | QC           | 23            | 0       | QC    | 5975CACQF.M     |

## Quantitation Results

### Compound: Dichlorodifluoromethane

| Data File | Sample Type | ISTD          | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Fluorobenzene |       |        | 775552    |            | ND         |           |          |
| 04JAN10.D | Calibration | Fluorobenzene | 1.241 | 4353   | 770895    | 0.0056     | 4.3090     | 2.5000    | 172.4    |
| 04JAN11.D | Calibration | Fluorobenzene | 1.244 | 12087  | 764419    | 0.0158     | 12.0663    | 12.5000   | 96.5     |
| 04JAN12.D | Calibration | Fluorobenzene | 1.244 | 26627  | 791270    | 0.0337     | 25.6793    | 25.0000   | 102.7    |
| 04JAN13.D | Calibration | Fluorobenzene | 1.241 | 50457  | 778120    | 0.0648     | 49.4835    | 50.0000   | 99.0     |
| 04JAN15.D | Calibration | Fluorobenzene | 1.241 | 137933 | 823488    | 0.1675     | 127.8193   | 125.0000  | 102.3    |
| 04JAN17.D | Calibration | Fluorobenzene | 1.241 | 276334 | 836278    | 0.3304     | 252.1559   | 250.0000  | 100.9    |
| 04JAN19.D | Calibration | Fluorobenzene | 1.241 | 412544 | 841876    | 0.4900     | 373.9449   | 375.0000  | 99.7     |
| 04JAN21.D | Calibration | Fluorobenzene | 1.241 | 545484 | 841364    | 0.6483     | 494.7474   | 500.0000  | 98.9     |
| 04JAN23.D | QC          | Fluorobenzene | 1.241 | 116936 | 801210    | 0.1459     | 111.3749   | 125.0000  |          |

### Compound: Chloromethane

| Data File | Sample Type | ISTD          | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Fluorobenzene | 1.333 | 0      | 775552    | 0.0000     | ND         |           |          |
| 04JAN10.D | Calibration | Fluorobenzene | 1.406 | 7435   | 770895    | 0.0096     | 6.0637     | 2.5000    | 242.5    |
| 04JAN11.D | Calibration | Fluorobenzene | 1.406 | 16859  | 764419    | 0.0221     | 13.8661    | 12.5000   | 110.9    |
| 04JAN12.D | Calibration | Fluorobenzene | 1.406 | 33153  | 791270    | 0.0419     | 26.3422    | 25.0000   | 105.4    |
| 04JAN13.D | Calibration | Fluorobenzene | 1.408 | 61632  | 778120    | 0.0792     | 49.7983    | 50.0000   | 99.6     |
| 04JAN15.D | Calibration | Fluorobenzene | 1.409 | 160604 | 823488    | 0.1950     | 122.6179   | 125.0000  | 98.1     |
| 04JAN17.D | Calibration | Fluorobenzene | 1.408 | 319523 | 836278    | 0.3821     | 240.2183   | 250.0000  | 96.1     |
| 04JAN19.D | Calibration | Fluorobenzene | 1.409 | 471454 | 841876    | 0.5600     | 352.0836   | 375.0000  | 93.9     |
| 04JAN21.D | Calibration | Fluorobenzene | 1.406 | 642582 | 841364    | 0.7637     | 480.1747   | 500.0000  | 96.0     |

# Quantitative Analysis Results Summary Report

**Compound: Chloromethane**

| Data File | Sample Type | ISTD          | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN23.D | QC          | Fluorobenzene | 1.406 | 138617 | 801210    | 0.1730     | 108.7739   | 125.0000  |          |

**Compound: Vinyl chloride**

| Data File | Sample Type | ISTD          | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Fluorobenzene | 1.489 | 0      | 775552    | 0.0000     | ND         |           |          |
| 04JAN10.D | Calibration | Fluorobenzene | 1.495 | 4274   | 770895    | 0.0055     | 3.8739     | 2.5000    | 155.0    |
| 04JAN11.D | Calibration | Fluorobenzene | 1.498 | 13724  | 764419    | 0.0180     | 12.5446    | 12.5000   | 100.4    |
| 04JAN12.D | Calibration | Fluorobenzene | 1.495 | 29046  | 791270    | 0.0367     | 25.6488    | 25.0000   | 102.6    |
| 04JAN13.D | Calibration | Fluorobenzene | 1.495 | 54521  | 778120    | 0.0701     | 48.9580    | 50.0000   | 97.9     |
| 04JAN15.D | Calibration | Fluorobenzene | 1.495 | 148358 | 823488    | 0.1802     | 125.8809   | 125.0000  | 100.7    |
| 04JAN17.D | Calibration | Fluorobenzene | 1.498 | 297604 | 836278    | 0.3559     | 248.6532   | 250.0000  | 99.5     |
| 04JAN19.D | Calibration | Fluorobenzene | 1.498 | 448643 | 841876    | 0.5329     | 372.3564   | 375.0000  | 99.3     |
| 04JAN21.D | Calibration | Fluorobenzene | 1.495 | 600092 | 841364    | 0.7132     | 498.3563   | 500.0000  | 99.7     |
| 04JAN23.D | QC          | Fluorobenzene | 1.495 | 137775 | 801210    | 0.1720     | 120.1518   | 125.0000  |          |

**Compound: Bromomethane**

| Data File | Sample Type | ISTD          | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Fluorobenzene |       |        | 775552    |            | ND         |           |          |
| 04JAN10.D | Calibration | Fluorobenzene | 1.796 | 1902   | 770895    | 0.0025     | 3.8547     | 2.5000    | 154.2    |
| 04JAN11.D | Calibration | Fluorobenzene | 1.796 | 5893   | 764419    | 0.0077     | 12.0464    | 12.5000   | 96.4     |
| 04JAN12.D | Calibration | Fluorobenzene | 1.796 | 13054  | 791270    | 0.0165     | 25.7793    | 25.0000   | 103.1    |
| 04JAN13.D | Calibration | Fluorobenzene | 1.799 | 23699  | 778120    | 0.0305     | 47.5921    | 50.0000   | 95.2     |
| 04JAN15.D | Calibration | Fluorobenzene | 1.799 | 65163  | 823488    | 0.0791     | 123.6504   | 125.0000  | 98.9     |
| 04JAN17.D | Calibration | Fluorobenzene | 1.799 | 134737 | 836278    | 0.1611     | 251.7606   | 250.0000  | 100.7    |
| 04JAN19.D | Calibration | Fluorobenzene | 1.796 | 207491 | 841876    | 0.2465     | 385.1259   | 375.0000  | 102.7    |
| 04JAN21.D | Calibration | Fluorobenzene | 1.793 | 277301 | 841364    | 0.3296     | 515.0141   | 500.0000  | 103.0    |
| 04JAN23.D | QC          | Fluorobenzene | 1.796 | 59947  | 801210    | 0.0748     | 116.9157   | 125.0000  |          |

**Compound: Chloroethane**

| Data File | Sample Type | ISTD          | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Fluorobenzene |       |        | 775552    |            | ND         |           |          |
| 04JAN10.D | Calibration | Fluorobenzene | 1.899 | 2178   | 770895    | 0.0028     | 3.9871     | 2.5000    | 159.5    |
| 04JAN11.D | Calibration | Fluorobenzene | 1.897 | 8052   | 764419    | 0.0105     | 14.8670    | 12.5000   | 118.9    |
| 04JAN12.D | Calibration | Fluorobenzene | 1.897 | 14646  | 791270    | 0.0185     | 26.1250    | 25.0000   | 104.5    |
| 04JAN13.D | Calibration | Fluorobenzene | 1.897 | 25484  | 778120    | 0.0328     | 46.2243    | 50.0000   | 92.4     |
| 04JAN15.D | Calibration | Fluorobenzene | 1.894 | 71420  | 823488    | 0.0867     | 122.4086   | 125.0000  | 97.9     |
| 04JAN17.D | Calibration | Fluorobenzene | 1.894 | 137312 | 836278    | 0.1642     | 231.7432   | 250.0000  | 92.7     |
| 04JAN19.D | Calibration | Fluorobenzene | 1.897 | 217393 | 841876    | 0.2582     | 364.4573   | 375.0000  | 97.2     |
| 04JAN21.D | Calibration | Fluorobenzene | 1.894 | 287041 | 841364    | 0.3412     | 481.5143   | 500.0000  | 96.3     |
| 04JAN23.D | QC          | Fluorobenzene | 1.897 | 65619  | 801210    | 0.0819     | 115.5932   | 125.0000  |          |

# Quantitative Analysis Results Summary Report

**Compound: Trichlorofluoromethane**

| Data File | Sample Type | ISTD          | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Fluorobenzene |       |        | 775552    |            | ND         |           |          |
| 04JAN10.D | Calibration | Fluorobenzene | 2.153 | 5030   | 770895    | 0.0065     | 3.6731     | 2.5000    | 146.9    |
| 04JAN11.D | Calibration | Fluorobenzene | 2.142 | 15431  | 764419    | 0.0202     | 11.3637    | 12.5000   | 90.9     |
| 04JAN12.D | Calibration | Fluorobenzene | 2.142 | 37464  | 791270    | 0.0473     | 26.6531    | 25.0000   | 106.6    |
| 04JAN13.D | Calibration | Fluorobenzene | 2.145 | 68163  | 778120    | 0.0876     | 49.3128    | 50.0000   | 98.6     |
| 04JAN15.D | Calibration | Fluorobenzene | 2.142 | 188808 | 823488    | 0.2293     | 129.0687   | 125.0000  | 103.3    |
| 04JAN17.D | Calibration | Fluorobenzene | 2.145 | 384837 | 836278    | 0.4602     | 259.0502   | 250.0000  | 103.6    |
| 04JAN19.D | Calibration | Fluorobenzene | 2.145 | 555477 | 841876    | 0.6598     | 371.4290   | 375.0000  | 99.0     |
| 04JAN21.D | Calibration | Fluorobenzene | 2.145 | 731829 | 841364    | 0.8698     | 489.6475   | 500.0000  | 97.9     |
| 04JAN23.D | QC          | Fluorobenzene | 2.145 | 173333 | 801210    | 0.2163     | 121.7847   | 125.0000  |          |

**Compound: 1,1-Dichloroethene**

| Data File | Sample Type | ISTD          | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Fluorobenzene |       |        | 775552    |            | ND         |           |          |
| 04JAN10.D | Calibration | Fluorobenzene | 2.700 | 2084   | 770895    | 0.0027     | 2.6839     | 2.5000    | 107.4    |
| 04JAN11.D | Calibration | Fluorobenzene | 2.700 | 9169   | 764419    | 0.0120     | 11.9081    | 12.5000   | 95.3     |
| 04JAN12.D | Calibration | Fluorobenzene | 2.700 | 20631  | 791270    | 0.0261     | 25.8849    | 25.0000   | 103.5    |
| 04JAN13.D | Calibration | Fluorobenzene | 2.702 | 38253  | 778120    | 0.0492     | 48.8056    | 50.0000   | 97.6     |
| 04JAN15.D | Calibration | Fluorobenzene | 2.697 | 99438  | 823488    | 0.1208     | 119.8798   | 125.0000  | 95.9     |
| 04JAN17.D | Calibration | Fluorobenzene | 2.702 | 217406 | 836278    | 0.2600     | 258.0903   | 250.0000  | 103.2    |
| 04JAN19.D | Calibration | Fluorobenzene | 2.700 | 322557 | 841876    | 0.3831     | 380.3725   | 375.0000  | 101.4    |
| 04JAN21.D | Calibration | Fluorobenzene | 2.700 | 436507 | 841364    | 0.5188     | 515.0603   | 500.0000  | 103.0    |
| 04JAN23.D | QC          | Fluorobenzene | 2.702 | 108512 | 801210    | 0.1354     | 134.4566   | 125.0000  |          |

**Compound: Methylene chloride**

| Data File | Sample Type | ISTD          | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Fluorobenzene | 3.335 | 1661   | 775552    | 0.0021     | 1.4424     |           |          |
| 04JAN10.D | Calibration | Fluorobenzene | 3.324 | 4095   | 770895    | 0.0053     | 3.5774     | 2.5000    | 143.1    |
| 04JAN11.D | Calibration | Fluorobenzene | 3.338 | 17734  | 764419    | 0.0232     | 15.6236    | 12.5000   | 125.0    |
| 04JAN12.D | Calibration | Fluorobenzene | 3.333 | 30908  | 791270    | 0.0391     | 26.3058    | 25.0000   | 105.2    |
| 04JAN13.D | Calibration | Fluorobenzene | 3.335 | 58282  | 778120    | 0.0749     | 50.4421    | 50.0000   | 100.9    |
| 04JAN15.D | Calibration | Fluorobenzene | 3.336 | 135271 | 823488    | 0.1643     | 110.6249   | 125.0000  | 88.5     |
| 04JAN17.D | Calibration | Fluorobenzene | 3.333 | 292397 | 836278    | 0.3496     | 235.4657   | 250.0000  | 94.2     |
| 04JAN19.D | Calibration | Fluorobenzene | 3.330 | 435116 | 841876    | 0.5168     | 348.0666   | 375.0000  | 92.8     |
| 04JAN21.D | Calibration | Fluorobenzene | 3.330 | 583438 | 841364    | 0.6934     | 466.9993   | 500.0000  | 93.4     |
| 04JAN23.D | QC          | Fluorobenzene | 3.330 | 144585 | 801210    | 0.1805     | 121.5297   | 125.0000  |          |

**Compound: trans-1,2-Dichloroethene**

| Data File | Sample Type | ISTD          | RT    | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Fluorobenzene |       |      | 775552    |            | ND         |           |          |
| 04JAN10.D | Calibration | Fluorobenzene | 3.723 | 2146 | 770895    | 0.0028     | 2.7090     | 2.5000    | 108.4    |
| 04JAN11.D | Calibration | Fluorobenzene | 3.720 | 9821 | 764419    | 0.0128     | 12.5022    | 12.5000   | 100.0    |

# Quantitative Analysis Results Summary Report

**Compound: trans-1,2-Dichloroethene**

| Data File | Sample Type | ISTD          | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN12.D | Calibration | Fluorobenzene | 3.712 | 20706  | 791270    | 0.0262     | 25.4641    | 25.0000   | 101.9    |
| 04JAN13.D | Calibration | Fluorobenzene | 3.717 | 39596  | 778120    | 0.0509     | 49.5178    | 50.0000   | 99.0     |
| 04JAN15.D | Calibration | Fluorobenzene | 3.718 | 100409 | 823488    | 0.1219     | 118.6511   | 125.0000  | 94.9     |
| 04JAN17.D | Calibration | Fluorobenzene | 3.715 | 218855 | 836278    | 0.2617     | 254.6608   | 250.0000  | 101.9    |
| 04JAN19.D | Calibration | Fluorobenzene | 3.715 | 325415 | 841876    | 0.3865     | 376.1367   | 375.0000  | 100.3    |
| 04JAN21.D | Calibration | Fluorobenzene | 3.718 | 440967 | 841364    | 0.5241     | 510.0097   | 500.0000  | 102.0    |
| 04JAN23.D | QC          | Fluorobenzene | 3.715 | 110909 | 801210    | 0.1384     | 134.7028   | 125.0000  |          |

**Compound: Methyl tert-butyl ether (MTBE)**

| Data File | Sample Type | ISTD          | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Fluorobenzene |       |        | 775552    |            | ND         |           |          |
| 04JAN10.D | Calibration | Fluorobenzene | 3.759 | 2717   | 770895    | 0.0035     | 2.6532     | 2.5000    | 106.1    |
| 04JAN11.D | Calibration | Fluorobenzene | 3.762 | 12515  | 764419    | 0.0164     | 12.3255    | 12.5000   | 98.6     |
| 04JAN12.D | Calibration | Fluorobenzene | 3.754 | 24218  | 791270    | 0.0306     | 23.0418    | 25.0000   | 92.2     |
| 04JAN13.D | Calibration | Fluorobenzene | 3.757 | 49126  | 778120    | 0.0631     | 47.5301    | 50.0000   | 95.1     |
| 04JAN15.D | Calibration | Fluorobenzene | 3.754 | 139068 | 823488    | 0.1689     | 127.1375   | 125.0000  | 101.7    |
| 04JAN17.D | Calibration | Fluorobenzene | 3.751 | 287653 | 836278    | 0.3440     | 258.9535   | 250.0000  | 103.6    |
| 04JAN19.D | Calibration | Fluorobenzene | 3.751 | 437439 | 841876    | 0.5196     | 391.1767   | 375.0000  | 104.3    |
| 04JAN21.D | Calibration | Fluorobenzene | 3.754 | 584294 | 841364    | 0.6945     | 522.8187   | 500.0000  | 104.6    |
| 04JAN23.D | QC          | Fluorobenzene | 3.754 | 143378 | 801210    | 0.1790     | 134.7224   | 125.0000  |          |

**Compound: 1,1-Dichloroethane**

| Data File | Sample Type | ISTD          | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Fluorobenzene |       |        | 775552    |            | ND         |           |          |
| 04JAN10.D | Calibration | Fluorobenzene | 4.376 | 3892   | 770895    | 0.0050     | 2.6393     | 2.5000    | 105.6    |
| 04JAN11.D | Calibration | Fluorobenzene | 4.378 | 17642  | 764419    | 0.0231     | 12.0652    | 12.5000   | 96.5     |
| 04JAN12.D | Calibration | Fluorobenzene | 4.379 | 38874  | 791270    | 0.0491     | 25.6835    | 25.0000   | 102.7    |
| 04JAN13.D | Calibration | Fluorobenzene | 4.381 | 73205  | 778120    | 0.0941     | 49.1828    | 50.0000   | 98.4     |
| 04JAN15.D | Calibration | Fluorobenzene | 4.378 | 186052 | 823488    | 0.2259     | 118.1125   | 125.0000  | 94.5     |
| 04JAN17.D | Calibration | Fluorobenzene | 4.384 | 413408 | 836278    | 0.4943     | 258.4325   | 250.0000  | 103.4    |
| 04JAN19.D | Calibration | Fluorobenzene | 4.381 | 612660 | 841876    | 0.7277     | 380.4437   | 375.0000  | 101.5    |
| 04JAN21.D | Calibration | Fluorobenzene | 4.378 | 829359 | 841364    | 0.9857     | 515.3207   | 500.0000  | 103.1    |
| 04JAN23.D | QC          | Fluorobenzene | 4.376 | 208131 | 801210    | 0.2598     | 135.8030   | 125.0000  |          |

**Compound: 2,2-Dichloropropane**

| Data File | Sample Type | ISTD          | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Fluorobenzene |       |        | 775552    |            | ND         |           |          |
| 04JAN10.D | Calibration | Fluorobenzene | 5.196 | 2930   | 770895    | 0.0038     | 2.6520     | 2.5000    | 106.1    |
| 04JAN11.D | Calibration | Fluorobenzene | 5.196 | 13676  | 764419    | 0.0179     | 12.4820    | 12.5000   | 99.9     |
| 04JAN12.D | Calibration | Fluorobenzene | 5.190 | 29793  | 791270    | 0.0377     | 26.2692    | 25.0000   | 105.1    |
| 04JAN13.D | Calibration | Fluorobenzene | 5.193 | 56189  | 778120    | 0.0722     | 50.3804    | 50.0000   | 100.8    |
| 04JAN15.D | Calibration | Fluorobenzene | 5.196 | 139656 | 823488    | 0.1696     | 118.3203   | 125.0000  | 94.7     |

# Quantitative Analysis Results Summary Report

**Compound: 2,2-Dichloropropane**

| Data File | Sample Type | ISTD          | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN17.D | Calibration | Fluorobenzene | 5.190 | 303307 | 836278    | 0.3627     | 253.0397   | 250.0000  | 101.2    |
| 04JAN19.D | Calibration | Fluorobenzene | 5.190 | 446282 | 841876    | 0.5301     | 369.8436   | 375.0000  | 98.6     |
| 04JAN21.D | Calibration | Fluorobenzene | 5.190 | 601823 | 841364    | 0.7153     | 499.0473   | 500.0000  | 99.8     |
| 04JAN23.D | QC          | Fluorobenzene | 5.190 | 150902 | 801210    | 0.1883     | 131.4031   | 125.0000  |          |

**Compound: cis-1,2-Dichloroethene**

| Data File | Sample Type | ISTD          | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Fluorobenzene |       |        | 775552    |            | ND         |           |          |
| 04JAN10.D | Calibration | Fluorobenzene | 5.212 | 2376   | 770895    | 0.0031     | 2.9581     | 2.5000    | 118.3    |
| 04JAN11.D | Calibration | Fluorobenzene | 5.221 | 10008  | 764419    | 0.0131     | 12.5659    | 12.5000   | 100.5    |
| 04JAN12.D | Calibration | Fluorobenzene | 5.212 | 20252  | 791270    | 0.0256     | 24.5653    | 25.0000   | 98.3     |
| 04JAN13.D | Calibration | Fluorobenzene | 5.209 | 39251  | 778120    | 0.0504     | 48.4154    | 50.0000   | 96.8     |
| 04JAN15.D | Calibration | Fluorobenzene | 5.215 | 100057 | 823488    | 0.1215     | 116.6190   | 125.0000  | 93.3     |
| 04JAN17.D | Calibration | Fluorobenzene | 5.215 | 228170 | 836278    | 0.2728     | 261.8706   | 250.0000  | 104.7    |
| 04JAN19.D | Calibration | Fluorobenzene | 5.212 | 339211 | 841876    | 0.4029     | 386.7236   | 375.0000  | 103.1    |
| 04JAN21.D | Calibration | Fluorobenzene | 5.212 | 452377 | 841364    | 0.5377     | 516.0544   | 500.0000  | 103.2    |
| 04JAN23.D | QC          | Fluorobenzene | 5.209 | 108623 | 801210    | 0.1356     | 130.1231   | 125.0000  |          |

**Compound: Methyl ethyl ketone**

| Data File | Sample Type | ISTD          | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Fluorobenzene |       |        | 775552    |            | ND         |           |          |
| 04JAN10.D | Calibration | Fluorobenzene | 5.302 | 3035   | 770895    | 0.0039     | 27.8967    | 25.0000   | 111.6    |
| 04JAN11.D | Calibration | Fluorobenzene | 5.288 | 13167  | 764419    | 0.0172     | 122.0520   | 125.0000  | 97.6     |
| 04JAN12.D | Calibration | Fluorobenzene | 5.282 | 26248  | 791270    | 0.0332     | 235.0504   | 250.0000  | 94.0     |
| 04JAN13.D | Calibration | Fluorobenzene | 5.285 | 52648  | 778120    | 0.0677     | 479.4296   | 500.0000  | 95.9     |
| 04JAN15.D | Calibration | Fluorobenzene | 5.282 | 134730 | 823488    | 0.1636     | 1159.3019  | 1250.0000 | 92.7     |
| 04JAN17.D | Calibration | Fluorobenzene | 5.279 | 317271 | 836278    | 0.3794     | 2688.2474  | 2500.0000 | 107.5    |
| 04JAN19.D | Calibration | Fluorobenzene | 5.279 | 470653 | 841876    | 0.5591     | 3961.3410  | 3750.0000 | 105.6    |
| 04JAN21.D | Calibration | Fluorobenzene | 5.279 | 632539 | 841364    | 0.7518     | 5327.1253  | 5000.0000 | 106.5    |
| 04JAN23.D | QC          | Fluorobenzene | 5.282 | 135511 | 801210    | 0.1691     | 1198.4439  | 1250.0000 |          |

**Compound: Bromochloromethane**

| Data File | Sample Type | ISTD          | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Fluorobenzene |       |        | 775552    |            | ND         |           |          |
| 04JAN10.D | Calibration | Fluorobenzene | 5.522 | 807    | 770895    | 0.0010     | 2.4260     | 2.5000    | 97.0     |
| 04JAN11.D | Calibration | Fluorobenzene | 5.516 | 4275   | 764419    | 0.0056     | 12.9568    | 12.5000   | 103.7    |
| 04JAN12.D | Calibration | Fluorobenzene | 5.522 | 8688   | 791270    | 0.0110     | 25.4383    | 25.0000   | 101.8    |
| 04JAN13.D | Calibration | Fluorobenzene | 5.516 | 17338  | 778120    | 0.0223     | 51.6233    | 50.0000   | 103.2    |
| 04JAN15.D | Calibration | Fluorobenzene | 5.519 | 41966  | 823488    | 0.0510     | 118.0683   | 125.0000  | 94.5     |
| 04JAN17.D | Calibration | Fluorobenzene | 5.519 | 89178  | 836278    | 0.1066     | 247.0586   | 250.0000  | 98.8     |
| 04JAN19.D | Calibration | Fluorobenzene | 5.516 | 135103 | 841876    | 0.1605     | 371.8004   | 375.0000  | 99.1     |
| 04JAN21.D | Calibration | Fluorobenzene | 5.519 | 179618 | 841364    | 0.2135     | 494.6054   | 500.0000  | 98.9     |

# Quantitative Analysis Results Summary Report

**Compound: Bromochloromethane**

| Data File | Sample Type | ISTD          | RT    | Resp  | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|-------|-----------|------------|------------|-----------|----------|
| 04JAN23.D | QC          | Fluorobenzene | 5.513 | 42744 | 801210    | 0.0533     | 123.6009   | 125.0000  |          |

**Compound: Chloroform**

| Data File | Sample Type | ISTD          | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Fluorobenzene |       |        | 775552    |            | ND         |           |          |
| 04JAN10.D | Calibration | Fluorobenzene | 5.659 | 4248   | 770895    | 0.0055     | 2.8946     | 2.5000    | 115.8    |
| 04JAN11.D | Calibration | Fluorobenzene | 5.656 | 19015  | 764419    | 0.0249     | 13.0668    | 12.5000   | 104.5    |
| 04JAN12.D | Calibration | Fluorobenzene | 5.653 | 36413  | 791270    | 0.0460     | 24.1734    | 25.0000   | 96.7     |
| 04JAN13.D | Calibration | Fluorobenzene | 5.650 | 71403  | 778120    | 0.0918     | 48.2031    | 50.0000   | 96.4     |
| 04JAN15.D | Calibration | Fluorobenzene | 5.653 | 179640 | 823488    | 0.2181     | 114.5912   | 125.0000  | 91.7     |
| 04JAN17.D | Calibration | Fluorobenzene | 5.653 | 394946 | 836278    | 0.4723     | 248.0804   | 250.0000  | 99.2     |
| 04JAN19.D | Calibration | Fluorobenzene | 5.650 | 588080 | 841876    | 0.6985     | 366.9389   | 375.0000  | 97.9     |
| 04JAN21.D | Calibration | Fluorobenzene | 5.653 | 783422 | 841364    | 0.9311     | 489.1221   | 500.0000  | 97.8     |
| 04JAN23.D | QC          | Fluorobenzene | 5.647 | 183676 | 801210    | 0.2292     | 120.4236   | 125.0000  |          |

**Compound: 1,1,1-Trichloroethane**

| Data File | Sample Type | ISTD          | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Fluorobenzene |       |        | 775552    |            | ND         |           |          |
| 04JAN10.D | Calibration | Fluorobenzene | 5.831 | 3510   | 770895    | 0.0046     | 2.5521     | 2.5000    | 102.1    |
| 04JAN11.D | Calibration | Fluorobenzene | 5.837 | 16623  | 764419    | 0.0217     | 12.1891    | 12.5000   | 97.5     |
| 04JAN12.D | Calibration | Fluorobenzene | 5.826 | 35547  | 791270    | 0.0449     | 25.1809    | 25.0000   | 100.7    |
| 04JAN13.D | Calibration | Fluorobenzene | 5.834 | 67007  | 778120    | 0.0861     | 48.2688    | 50.0000   | 96.5     |
| 04JAN15.D | Calibration | Fluorobenzene | 5.834 | 174206 | 823488    | 0.2115     | 118.5764   | 125.0000  | 94.9     |
| 04JAN17.D | Calibration | Fluorobenzene | 5.831 | 386005 | 836278    | 0.4616     | 258.7228   | 250.0000  | 103.5    |
| 04JAN19.D | Calibration | Fluorobenzene | 5.831 | 580748 | 841876    | 0.6898     | 386.6625   | 375.0000  | 103.1    |
| 04JAN21.D | Calibration | Fluorobenzene | 5.834 | 778785 | 841364    | 0.9256     | 518.8312   | 500.0000  | 103.8    |
| 04JAN23.D | QC          | Fluorobenzene | 5.831 | 183324 | 801210    | 0.2288     | 128.2524   | 125.0000  |          |

**Compound: Dibromofluoromethane**

| Data File | Sample Type | ISTD          | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Fluorobenzene | 5.848 | 203459 | 775552    | 0.2623     | 278.4635   |           |          |
| 04JAN10.D | Calibration | Fluorobenzene | 5.851 | 2508   | 770895    | 0.0033     | 3.4533     | 2.5000    | 138.1    |
| 04JAN11.D | Calibration | Fluorobenzene | 5.845 | 9074   | 764419    | 0.0119     | 12.6000    | 12.5000   | 100.8    |
| 04JAN12.D | Calibration | Fluorobenzene | 5.845 | 19100  | 791270    | 0.0241     | 25.6219    | 25.0000   | 102.5    |
| 04JAN13.D | Calibration | Fluorobenzene | 5.848 | 35309  | 778120    | 0.0454     | 48.1661    | 50.0000   | 96.3     |
| 04JAN15.D | Calibration | Fluorobenzene | 5.845 | 89307  | 823488    | 0.1084     | 115.1146   | 125.0000  | 92.1     |
| 04JAN17.D | Calibration | Fluorobenzene | 5.845 | 204073 | 836278    | 0.2440     | 259.0223   | 250.0000  | 103.6    |
| 04JAN19.D | Calibration | Fluorobenzene | 5.848 | 305158 | 841876    | 0.3625     | 384.7503   | 375.0000  | 102.6    |
| 04JAN21.D | Calibration | Fluorobenzene | 5.845 | 404568 | 841364    | 0.4808     | 510.3991   | 500.0000  | 102.1    |
| 04JAN23.D | QC          | Fluorobenzene | 5.848 | 204707 | 801210    | 0.2555     | 271.1994   | 250.0000  |          |



# Quantitative Analysis Results Summary Report

**Compound: Carbon tetrachloride**

| Data File | Sample Type | ISTD          | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Fluorobenzene |       |        | 775552    |            | ND         |           |          |
| 04JAN10.D | Calibration | Fluorobenzene | 6.029 | 4342   | 770895    | 0.0056     | 3.2043     | 2.5000    | 128.2    |
| 04JAN11.D | Calibration | Fluorobenzene | 6.021 | 16466  | 764419    | 0.0215     | 12.2545    | 12.5000   | 98.0     |
| 04JAN12.D | Calibration | Fluorobenzene | 6.024 | 34462  | 791270    | 0.0436     | 24.7773    | 25.0000   | 99.1     |
| 04JAN13.D | Calibration | Fluorobenzene | 6.026 | 65313  | 778120    | 0.0839     | 47.7520    | 50.0000   | 95.5     |
| 04JAN15.D | Calibration | Fluorobenzene | 6.024 | 172928 | 823488    | 0.2100     | 119.4667   | 125.0000  | 95.6     |
| 04JAN17.D | Calibration | Fluorobenzene | 6.026 | 383485 | 836278    | 0.4586     | 260.8774   | 250.0000  | 104.4    |
| 04JAN19.D | Calibration | Fluorobenzene | 6.024 | 572545 | 841876    | 0.6801     | 386.9014   | 375.0000  | 103.2    |
| 04JAN21.D | Calibration | Fluorobenzene | 6.024 | 770907 | 841364    | 0.9163     | 521.2630   | 500.0000  | 104.3    |
| 04JAN23.D | QC          | Fluorobenzene | 6.027 | 181384 | 801210    | 0.2264     | 128.7928   | 125.0000  |          |

**Compound: 1,1-Dichloropropene**

| Data File | Sample Type | ISTD          | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Fluorobenzene |       |        | 775552    |            | ND         |           |          |
| 04JAN10.D | Calibration | Fluorobenzene | 6.041 | 2830   | 770895    | 0.0037     | 2.4201     | 2.5000    | 96.8     |
| 04JAN11.D | Calibration | Fluorobenzene | 6.038 | 13149  | 764419    | 0.0172     | 11.3397    | 12.5000   | 90.7     |
| 04JAN12.D | Calibration | Fluorobenzene | 6.038 | 29241  | 791270    | 0.0370     | 24.3617    | 25.0000   | 97.4     |
| 04JAN13.D | Calibration | Fluorobenzene | 6.035 | 56376  | 778120    | 0.0725     | 47.7627    | 50.0000   | 95.5     |
| 04JAN15.D | Calibration | Fluorobenzene | 6.038 | 149649 | 823488    | 0.1817     | 119.8002   | 125.0000  | 95.8     |
| 04JAN17.D | Calibration | Fluorobenzene | 6.038 | 335741 | 836278    | 0.4015     | 264.6638   | 250.0000  | 105.9    |
| 04JAN19.D | Calibration | Fluorobenzene | 6.040 | 507157 | 841876    | 0.6024     | 397.1322   | 375.0000  | 105.9    |
| 04JAN21.D | Calibration | Fluorobenzene | 6.038 | 693669 | 841364    | 0.8245     | 543.5121   | 500.0000  | 108.7    |
| 04JAN23.D | QC          | Fluorobenzene | 6.038 | 150930 | 801210    | 0.1884     | 124.1853   | 125.0000  |          |

**Compound: 1,2-Dichloroethane-d4**

| Data File | Sample Type | ISTD          | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Fluorobenzene | 6.233 | 88174  | 775552    | 0.1137     | 279.3964   |           |          |
| 04JAN10.D | Calibration | Fluorobenzene | 6.233 | 923    | 770895    | 0.0012     | 2.9438     | 2.5000    | 117.8    |
| 04JAN11.D | Calibration | Fluorobenzene | 6.227 | 3938   | 764419    | 0.0052     | 12.6600    | 12.5000   | 101.3    |
| 04JAN12.D | Calibration | Fluorobenzene | 6.236 | 8284   | 791270    | 0.0105     | 25.7280    | 25.0000   | 102.9    |
| 04JAN13.D | Calibration | Fluorobenzene | 6.233 | 15238  | 778120    | 0.0196     | 48.1252    | 50.0000   | 96.3     |
| 04JAN15.D | Calibration | Fluorobenzene | 6.233 | 39086  | 823488    | 0.0475     | 116.6420   | 125.0000  | 93.3     |
| 04JAN17.D | Calibration | Fluorobenzene | 6.236 | 87876  | 836278    | 0.1051     | 258.2324   | 250.0000  | 103.3    |
| 04JAN19.D | Calibration | Fluorobenzene | 6.233 | 129608 | 841876    | 0.1540     | 378.3335   | 375.0000  | 100.9    |
| 04JAN21.D | Calibration | Fluorobenzene | 6.233 | 174713 | 841364    | 0.2077     | 510.3080   | 500.0000  | 102.1    |
| 04JAN23.D | QC          | Fluorobenzene | 6.230 | 91382  | 801210    | 0.1141     | 280.2886   | 250.0000  |          |

**Compound: Benzene**

| Data File | Sample Type | ISTD          | RT    | Resp  | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|-------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Fluorobenzene | 6.266 | 381   | 775552    | 0.0005     | 0.1233     |           |          |
| 04JAN10.D | Calibration | Fluorobenzene | 6.278 | 8408  | 770895    | 0.0109     | 2.7393     | 2.5000    | 109.6    |
| 04JAN11.D | Calibration | Fluorobenzene | 6.278 | 37071 | 764419    | 0.0485     | 12.1801    | 12.5000   | 97.4     |

# Quantitative Analysis Results Summary Report

**Compound: Benzene**

| Data File | Sample Type | ISTD          | RT    | Resp    | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|---------|-----------|------------|------------|-----------|----------|
| 04JAN12.D | Calibration | Fluorobenzene | 6.278 | 74956   | 791270    | 0.0947     | 23.7919    | 25.0000   | 95.2     |
| 04JAN13.D | Calibration | Fluorobenzene | 6.277 | 148727  | 778120    | 0.1911     | 48.0054    | 50.0000   | 96.0     |
| 04JAN15.D | Calibration | Fluorobenzene | 6.278 | 383469  | 823488    | 0.4657     | 116.9553   | 125.0000  | 93.6     |
| 04JAN17.D | Calibration | Fluorobenzene | 6.280 | 857534  | 836278    | 1.0254     | 257.5416   | 250.0000  | 103.0    |
| 04JAN19.D | Calibration | Fluorobenzene | 6.278 | 1293370 | 841876    | 1.5363     | 385.8526   | 375.0000  | 102.9    |
| 04JAN21.D | Calibration | Fluorobenzene | 6.280 | 1714050 | 841364    | 2.0372     | 511.6658   | 500.0000  | 102.3    |
| 04JAN23.D | QC          | Fluorobenzene | 6.280 | 418900  | 801210    | 0.5228     | 131.3139   | 125.0000  |          |

**Compound: 1,2-Dichloroethane**

| Data File | Sample Type | ISTD          | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|---------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Fluorobenzene |       |        | 775552    |            | ND         |           |          |
| 04JAN10.D | Calibration | Fluorobenzene | 6.322 | 2415   | 770895    | 0.0031     | 2.9090     | 2.5000    | 116.4    |
| 04JAN11.D | Calibration | Fluorobenzene | 6.322 | 10202  | 764419    | 0.0133     | 12.3906    | 12.5000   | 99.1     |
| 04JAN12.D | Calibration | Fluorobenzene | 6.322 | 19996  | 791270    | 0.0253     | 23.4616    | 25.0000   | 93.8     |
| 04JAN13.D | Calibration | Fluorobenzene | 6.325 | 41058  | 778120    | 0.0528     | 48.9880    | 50.0000   | 98.0     |
| 04JAN15.D | Calibration | Fluorobenzene | 6.322 | 104855 | 823488    | 0.1273     | 118.2143   | 125.0000  | 94.6     |
| 04JAN17.D | Calibration | Fluorobenzene | 6.322 | 226964 | 836278    | 0.2714     | 251.9675   | 250.0000  | 100.8    |
| 04JAN19.D | Calibration | Fluorobenzene | 6.322 | 332775 | 841876    | 0.3953     | 366.9787   | 375.0000  | 97.9     |
| 04JAN21.D | Calibration | Fluorobenzene | 6.322 | 450739 | 841364    | 0.5357     | 497.3699   | 500.0000  | 99.5     |
| 04JAN23.D | QC          | Fluorobenzene | 6.325 | 104249 | 801210    | 0.1301     | 120.7991   | 125.0000  |          |

**Compound: Trichloroethene**

| Data File | Sample Type | ISTD             | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Chlorobenzene-d5 |       |        | 301196    |            | ND         |           |          |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 7.033 | 2372   | 296081    | 0.0080     | 2.6564     | 2.5000    | 106.3    |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 7.025 | 10442  | 296554    | 0.0352     | 11.6753    | 12.5000   | 93.4     |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 7.028 | 21946  | 301338    | 0.0728     | 24.1484    | 25.0000   | 96.6     |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 7.030 | 42682  | 300356    | 0.1421     | 47.1189    | 50.0000   | 94.2     |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 7.030 | 114123 | 306491    | 0.3724     | 123.4646   | 125.0000  | 98.8     |
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 7.030 | 250285 | 316399    | 0.7910     | 262.2931   | 250.0000  | 104.9    |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 7.028 | 374370 | 314668    | 1.1897     | 394.4896   | 375.0000  | 105.2    |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 7.028 | 505400 | 313585    | 1.6117     | 534.4007   | 500.0000  | 106.9    |
| 04JAN23.D | QC          | Chlorobenzene-d5 | 7.025 | 121734 | 307868    | 0.3954     | 131.1096   | 125.0000  |          |

**Compound: 1,2-Dichloropropane**

| Data File | Sample Type | ISTD             | RT    | Resp  | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|-------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Chlorobenzene-d5 |       |       | 301196    |            | ND         |           |          |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 7.273 | 2148  | 296081    | 0.0073     | 2.7347     | 2.5000    | 109.4    |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 7.270 | 9488  | 296554    | 0.0320     | 12.0602    | 12.5000   | 96.5     |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 7.270 | 20077 | 301338    | 0.0666     | 25.1147    | 25.0000   | 100.5    |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 7.273 | 37870 | 300356    | 0.1261     | 47.5273    | 50.0000   | 95.1     |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 7.270 | 99187 | 306491    | 0.3236     | 121.9890   | 125.0000  | 97.6     |

# Quantitative Analysis Results Summary Report

**Compound: 1,2-Dichloropropane**

| Data File | Sample Type | ISTD             | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 7.270 | 213800 | 316399    | 0.6757     | 254.7161   | 250.0000  | 101.9    |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 7.270 | 324602 | 314668    | 1.0316     | 388.8502   | 375.0000  | 103.7    |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 7.270 | 436057 | 313585    | 1.3906     | 524.1695   | 500.0000  | 104.8    |
| 04JAN23.D | QC          | Chlorobenzene-d5 | 7.270 | 102633 | 307868    | 0.3334     | 125.6626   | 125.0000  |          |

**Compound: Dibromomethane**

| Data File | Sample Type | ISTD             | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Chlorobenzene-d5 |       |        | 301196    |            | ND         |           |          |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 7.396 | 902    | 296081    | 0.0030     | 2.7162     | 2.5000    | 108.6    |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 7.399 | 4675   | 296554    | 0.0158     | 14.0619    | 12.5000   | 112.5    |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 7.393 | 8055   | 301338    | 0.0267     | 23.8439    | 25.0000   | 95.4     |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 7.396 | 15989  | 300356    | 0.0532     | 47.4844    | 50.0000   | 95.0     |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 7.399 | 40628  | 306491    | 0.1326     | 118.2425   | 125.0000  | 94.6     |
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 7.396 | 89483  | 316399    | 0.2828     | 252.2734   | 250.0000  | 100.9    |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 7.396 | 134282 | 314668    | 0.4267     | 380.6547   | 375.0000  | 101.5    |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 7.396 | 176038 | 313585    | 0.5614     | 500.7456   | 500.0000  | 100.1    |
| 04JAN23.D | QC          | Chlorobenzene-d5 | 7.393 | 43248  | 307868    | 0.1405     | 125.3047   | 125.0000  |          |

**Compound: Bromodichloromethane**

| Data File | Sample Type | ISTD             | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Chlorobenzene-d5 |       |        | 301196    |            | ND         |           |          |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 7.597 | 2536   | 296081    | 0.0086     | 2.7684     | 2.5000    | 110.7    |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 7.585 | 11562  | 296554    | 0.0390     | 12.6014    | 12.5000   | 100.8    |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 7.583 | 22743  | 301338    | 0.0755     | 24.3940    | 25.0000   | 97.6     |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 7.585 | 43900  | 300356    | 0.1462     | 47.2409    | 50.0000   | 94.5     |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 7.585 | 115664 | 306491    | 0.3774     | 121.9749   | 125.0000  | 97.6     |
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 7.582 | 251805 | 316399    | 0.7958     | 257.2286   | 250.0000  | 102.9    |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 7.585 | 375983 | 314668    | 1.1949     | 386.1940   | 375.0000  | 103.0    |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 7.585 | 502929 | 313585    | 1.6038     | 518.3718   | 500.0000  | 103.7    |
| 04JAN23.D | QC          | Chlorobenzene-d5 | 7.585 | 122757 | 307868    | 0.3987     | 128.8759   | 125.0000  |          |

**Compound: cis-1,3-Dichloropropene**

| Data File | Sample Type | ISTD             | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Chlorobenzene-d5 |       |        | 301196    |            | ND         |           |          |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 8.054 | 2583   | 296081    | 0.0087     | 2.4939     | 2.5000    | 99.8     |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 8.062 | 12525  | 296554    | 0.0422     | 12.0738    | 12.5000   | 96.6     |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 8.057 | 24511  | 301338    | 0.0813     | 23.2528    | 25.0000   | 93.0     |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 8.057 | 48886  | 300356    | 0.1628     | 46.5283    | 50.0000   | 93.1     |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 8.059 | 129419 | 306491    | 0.4223     | 120.7116   | 125.0000  | 96.6     |
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 8.057 | 293617 | 316399    | 0.9280     | 265.2863   | 250.0000  | 106.1    |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 8.057 | 441168 | 314668    | 1.4020     | 400.7930   | 375.0000  | 106.9    |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 8.059 | 591147 | 313585    | 1.8851     | 538.9008   | 500.0000  | 107.8    |

# Quantitative Analysis Results Summary Report

**Compound: cis-1,3-Dichloropropene**

| Data File | Sample Type | ISTD             | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN23.D | QC          | Chlorobenzene-d5 | 8.054 | 130910 | 307868    | 0.4252     | 121.5561   | 125.0000  |          |

**Compound: Toluene-d8**

| Data File | Sample Type | ISTD             | RT    | Resp    | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|---------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Chlorobenzene-d5 | 8.319 | 770154  | 301196    | 2.5570     | 265.3436   |           |          |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 8.322 | 7777    | 296081    | 0.0263     | 2.7257     | 2.5000    | 109.0    |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 8.322 | 32318   | 296554    | 0.1090     | 11.3089    | 12.5000   | 90.5     |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 8.319 | 67673   | 301338    | 0.2246     | 23.3046    | 25.0000   | 93.2     |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 8.319 | 136453  | 300356    | 0.4543     | 47.1441    | 50.0000   | 94.3     |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 8.319 | 358186  | 306491    | 1.1687     | 121.2749   | 125.0000  | 97.0     |
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 8.319 | 823306  | 316399    | 2.6021     | 270.0265   | 250.0000  | 108.0    |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 8.322 | 1229775 | 314668    | 3.9082     | 405.5583   | 375.0000  | 108.1    |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 8.319 | 1644540 | 313585    | 5.2443     | 544.2136   | 500.0000  | 108.8    |
| 04JAN23.D | QC          | Chlorobenzene-d5 | 8.322 | 821531  | 307868    | 2.6685     | 276.9106   | 250.0000  |          |

**Compound: Toluene**

| Data File | Sample Type | ISTD             | RT    | Resp    | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|---------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Chlorobenzene-d5 |       |         | 301196    |            | ND         |           |          |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 8.380 | 5039    | 296081    | 0.0170     | 2.6145     | 2.5000    | 104.6    |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 8.388 | 21794   | 296554    | 0.0735     | 11.2899    | 12.5000   | 90.3     |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 8.389 | 46355   | 301338    | 0.1538     | 23.6319    | 25.0000   | 94.5     |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 8.388 | 91915   | 300356    | 0.3060     | 47.0116    | 50.0000   | 94.0     |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 8.389 | 244712  | 306491    | 0.7984     | 122.6571   | 125.0000  | 98.1     |
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 8.386 | 541945  | 316399    | 1.7129     | 263.1330   | 250.0000  | 105.3    |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 8.388 | 813204  | 314668    | 2.5843     | 397.0106   | 375.0000  | 105.9    |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 8.389 | 1095161 | 313585    | 3.4924     | 536.5101   | 500.0000  | 107.3    |
| 04JAN23.D | QC          | Chlorobenzene-d5 | 8.386 | 264584  | 307868    | 0.8594     | 132.0244   | 125.0000  |          |

**Compound: trans-1,3-Dichloropropene**

| Data File | Sample Type | ISTD             | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Chlorobenzene-d5 |       |        | 301196    |            | ND         |           |          |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 8.634 | 1470   | 296081    | 0.0050     | 1.9942     | 2.5000    | 79.8     |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 8.645 | 8683   | 296554    | 0.0293     | 11.7589    | 12.5000   | 94.1     |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 8.634 | 17850  | 301338    | 0.0592     | 23.7894    | 25.0000   | 95.2     |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 8.639 | 35179  | 300356    | 0.1171     | 47.0378    | 50.0000   | 94.1     |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 8.637 | 92719  | 306491    | 0.3025     | 121.4929   | 125.0000  | 97.2     |
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 8.639 | 207833 | 316399    | 0.6569     | 263.8027   | 250.0000  | 105.5    |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 8.639 | 315063 | 314668    | 1.0013     | 402.1098   | 375.0000  | 107.2    |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 8.637 | 416771 | 313585    | 1.3291     | 533.7551   | 500.0000  | 106.8    |
| 04JAN23.D | QC          | Chlorobenzene-d5 | 8.637 | 98907  | 307868    | 0.3213     | 129.0216   | 125.0000  |          |

# Quantitative Analysis Results Summary Report

## Compound: 1,1,2-Trichloroethane

| Data File | Sample Type | ISTD             | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Chlorobenzene-d5 |       |        | 301196    |            | ND         |           |          |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 8.810 | 960    | 296081    | 0.0032     | 2.5012     | 2.5000    | 100.0    |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 8.824 | 5090   | 296554    | 0.0172     | 13.2340    | 12.5000   | 105.9    |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 8.815 | 10099  | 301338    | 0.0335     | 25.8400    | 25.0000   | 103.4    |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 8.815 | 18884  | 300356    | 0.0629     | 48.4759    | 50.0000   | 97.0     |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 8.818 | 46673  | 306491    | 0.1523     | 117.4130   | 125.0000  | 93.9     |
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 8.815 | 101888 | 316399    | 0.3220     | 248.2882   | 250.0000  | 99.3     |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 8.818 | 152331 | 314668    | 0.4841     | 373.2534   | 375.0000  | 99.5     |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 8.815 | 205463 | 313585    | 0.6552     | 505.1803   | 500.0000  | 101.0    |
| 04JAN23.D | QC          | Chlorobenzene-d5 | 8.815 | 49128  | 307868    | 0.1596     | 123.0361   | 125.0000  |          |

## Compound: Tetrachloroethene

| Data File | Sample Type | ISTD             | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Chlorobenzene-d5 |       |        | 301196    |            | ND         |           |          |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 8.932 | 2105   | 296081    | 0.0071     | 2.6772     | 2.5000    | 107.1    |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 8.935 | 9238   | 296554    | 0.0312     | 11.7302    | 12.5000   | 93.8     |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 8.935 | 20322  | 301338    | 0.0674     | 25.3948    | 25.0000   | 101.6    |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 8.935 | 36925  | 300356    | 0.1229     | 46.2932    | 50.0000   | 92.6     |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 8.935 | 97590  | 306491    | 0.3184     | 119.9003   | 125.0000  | 95.9     |
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 8.938 | 218245 | 316399    | 0.6898     | 259.7419   | 250.0000  | 103.9    |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 8.938 | 319950 | 314668    | 1.0168     | 382.8796   | 375.0000  | 102.1    |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 8.938 | 428812 | 313585    | 1.3675     | 514.9255   | 500.0000  | 103.0    |
| 04JAN23.D | QC          | Chlorobenzene-d5 | 8.935 | 103027 | 307868    | 0.3346     | 126.0141   | 125.0000  |          |

## Compound: 1,3-Dichloropropane

| Data File | Sample Type | ISTD             | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Chlorobenzene-d5 |       |        | 301196    |            | ND         |           |          |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 8.977 | 2257   | 296081    | 0.0076     | 2.9881     | 2.5000    | 119.5    |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 8.985 | 8967   | 296554    | 0.0302     | 11.8526    | 12.5000   | 94.8     |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 8.983 | 18745  | 301338    | 0.0622     | 24.3839    | 25.0000   | 97.5     |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 8.980 | 37457  | 300356    | 0.1247     | 48.8841    | 50.0000   | 97.8     |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 8.980 | 96183  | 306491    | 0.3138     | 123.0132   | 125.0000  | 98.4     |
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 8.980 | 212669 | 316399    | 0.6722     | 263.4754   | 250.0000  | 105.4    |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 8.980 | 312547 | 314668    | 0.9933     | 389.3442   | 375.0000  | 103.8    |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 8.980 | 408993 | 313585    | 1.3042     | 511.2479   | 500.0000  | 102.2    |
| 04JAN23.D | QC          | Chlorobenzene-d5 | 8.980 | 95697  | 307868    | 0.3108     | 121.8442   | 125.0000  |          |

## Compound: Chlorodibromomethane

| Data File | Sample Type | ISTD             | RT    | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Chlorobenzene-d5 |       |      | 301196    |            | ND         |           |          |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 9.203 | 1468 | 296081    | 0.0050     | 2.4461     | 2.5000    | 97.8     |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 9.206 | 7718 | 296554    | 0.0260     | 12.8393    | 12.5000   | 102.7    |

# Quantitative Analysis Results Summary Report

**Compound: Chlorodibromomethane**

| Data File | Sample Type | ISTD             | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 9.197 | 14873  | 301338    | 0.0494     | 24.3492    | 25.0000   | 97.4     |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 9.203 | 28153  | 300356    | 0.0937     | 46.2411    | 50.0000   | 92.5     |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 9.206 | 75015  | 306491    | 0.2448     | 120.7454   | 125.0000  | 96.6     |
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 9.203 | 165695 | 316399    | 0.5237     | 258.3535   | 250.0000  | 103.3    |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 9.203 | 247279 | 314668    | 0.7858     | 387.6812   | 375.0000  | 103.4    |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 9.203 | 330813 | 313585    | 1.0549     | 520.4361   | 500.0000  | 104.1    |
| 04JAN23.D | QC          | Chlorobenzene-d5 | 9.203 | 78076  | 307868    | 0.2536     | 125.1103   | 125.0000  |          |

**Compound: 1,2-Dibromoethane**

| Data File | Sample Type | ISTD             | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Chlorobenzene-d5 |       |        | 301196    |            | ND         |           |          |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 9.300 | 1299   | 296081    | 0.0044     | 3.0943     | 2.5000    | 123.8    |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 9.300 | 5410   | 296554    | 0.0182     | 12.8640    | 12.5000   | 102.9    |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 9.309 | 10410  | 301338    | 0.0345     | 24.3601    | 25.0000   | 97.4     |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 9.303 | 21037  | 300356    | 0.0700     | 49.3889    | 50.0000   | 98.8     |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 9.306 | 51827  | 306491    | 0.1691     | 119.2394   | 125.0000  | 95.4     |
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 9.306 | 115714 | 316399    | 0.3657     | 257.8887   | 250.0000  | 103.2    |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 9.306 | 168577 | 314668    | 0.5357     | 377.7698   | 375.0000  | 100.7    |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 9.303 | 225877 | 313585    | 0.7203     | 507.9234   | 500.0000  | 101.6    |
| 04JAN23.D | QC          | Chlorobenzene-d5 | 9.306 | 54259  | 307868    | 0.1762     | 124.2764   | 125.0000  |          |

**Compound: Chlorobenzene**

| Data File | Sample Type | ISTD             | RT    | Resp    | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|---------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Chlorobenzene-d5 |       |         | 301196    |            | ND         |           |          |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 9.805 | 5771    | 296081    | 0.0195     | 2.7350     | 2.5000    | 109.4    |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 9.802 | 26461   | 296554    | 0.0892     | 12.5204    | 12.5000   | 100.2    |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 9.802 | 53047   | 301338    | 0.1760     | 24.7015    | 25.0000   | 98.8     |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 9.802 | 101452  | 300356    | 0.3378     | 47.3959    | 50.0000   | 94.8     |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 9.802 | 263617  | 306491    | 0.8601     | 120.6903   | 125.0000  | 96.6     |
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 9.802 | 582326  | 316399    | 1.8405     | 258.2544   | 250.0000  | 103.3    |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 9.802 | 867732  | 314668    | 2.7576     | 386.9455   | 375.0000  | 103.2    |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 9.802 | 1153147 | 313585    | 3.6773     | 515.9957   | 500.0000  | 103.2    |
| 04JAN23.D | QC          | Chlorobenzene-d5 | 9.802 | 288815  | 307868    | 0.9381     | 131.6352   | 125.0000  |          |

**Compound: 1,1,1,2-Tetrachloroethane**

| Data File | Sample Type | ISTD             | RT    | Resp  | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|-------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Chlorobenzene-d5 |       |       | 301196    |            | ND         |           |          |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 9.889 | 1893  | 296081    | 0.0064     | 2.5659     | 2.5000    | 102.6    |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 9.889 | 9473  | 296554    | 0.0319     | 12.8225    | 12.5000   | 102.6    |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 9.889 | 18130 | 301338    | 0.0602     | 24.1509    | 25.0000   | 96.6     |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 9.889 | 35544 | 300356    | 0.1183     | 47.5029    | 50.0000   | 95.0     |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 9.889 | 90898 | 306491    | 0.2966     | 119.0492   | 125.0000  | 95.2     |

# Quantitative Analysis Results Summary Report

**Compound: 1,1,1,2-Tetrachloroethane**

| Data File | Sample Type | ISTD             | RT    | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|--------|-----------|------------|------------|-----------|----------|
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 9.891 | 200859 | 316399    | 0.6348     | 254.8274   | 250.0000  | 101.9    |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 9.892 | 307436 | 314668    | 0.9770     | 392.1859   | 375.0000  | 104.6    |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 9.892 | 406450 | 313585    | 1.2961     | 520.2855   | 500.0000  | 104.1    |
| 04JAN23.D | QC          | Chlorobenzene-d5 | 9.892 | 97148  | 307868    | 0.3156     | 126.6657   | 125.0000  |          |

**Compound: Ethylbenzene**

| Data File | Sample Type | ISTD             | RT    | Resp    | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|-------|---------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Chlorobenzene-d5 |       |         | 301196    |            | ND         |           |          |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 9.920 | 9283    | 296081    | 0.0314     | 2.5367     | 2.5000    | 101.5    |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 9.917 | 40470   | 296554    | 0.1365     | 11.0411    | 12.5000   | 88.3     |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 9.917 | 88428   | 301338    | 0.2935     | 23.7421    | 25.0000   | 95.0     |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 9.917 | 173769  | 300356    | 0.5785     | 46.8079    | 50.0000   | 93.6     |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 9.920 | 464148  | 306491    | 1.5144     | 122.5243   | 125.0000  | 98.0     |
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 9.919 | 1043443 | 316399    | 3.2979     | 266.8193   | 250.0000  | 106.7    |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 9.919 | 1574219 | 314668    | 5.0028     | 404.7587   | 375.0000  | 107.9    |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 9.919 | 2111152 | 313585    | 6.7323     | 544.6881   | 500.0000  | 108.9    |
| 04JAN23.D | QC          | Chlorobenzene-d5 | 9.917 | 501953  | 307868    | 1.6304     | 131.9113   | 125.0000  |          |

**Compound: m+p-Xylenes**

| Data File | Sample Type | ISTD             | RT     | Resp    | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|--------|---------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Chlorobenzene-d5 |        |         | 301196    |            | ND         |           |          |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 10.045 | 7212    | 296081    | 0.0244     | 5.0712     | 5.0000    | 101.4    |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 10.037 | 31538   | 296554    | 0.1063     | 22.1410    | 25.0000   | 88.6     |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 10.039 | 66267   | 301338    | 0.2199     | 45.7836    | 50.0000   | 91.6     |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 10.039 | 133498  | 300356    | 0.4445     | 92.5347    | 100.0000  | 92.5     |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 10.039 | 368418  | 306491    | 1.2021     | 250.2587   | 250.0000  | 100.1    |
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 10.039 | 825866  | 316399    | 2.6102     | 543.4262   | 500.0000  | 108.7    |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 10.039 | 1228570 | 314668    | 3.9043     | 812.8556   | 750.0000  | 108.4    |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 10.039 | 1637879 | 313585    | 5.2231     | 1087.4082  | 1000.0000 | 108.7    |
| 04JAN23.D | QC          | Chlorobenzene-d5 | 10.039 | 388558  | 307868    | 1.2621     | 262.7589   | 250.0000  |          |

**Compound: o-Xylene**

| Data File | Sample Type | ISTD             | RT     | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|--------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Chlorobenzene-d5 |        |        | 301196    |            | ND         |           |          |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 10.430 | 3330   | 296081    | 0.0112     | 2.6303     | 2.5000    | 105.2    |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 10.430 | 13519  | 296554    | 0.0456     | 10.6612    | 12.5000   | 85.3     |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 10.427 | 30463  | 301338    | 0.1011     | 23.6420    | 25.0000   | 94.6     |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 10.430 | 61016  | 300356    | 0.2031     | 47.5086    | 50.0000   | 95.0     |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 10.430 | 161509 | 306491    | 0.5270     | 123.2378   | 125.0000  | 98.6     |
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 10.430 | 365914 | 316399    | 1.1565     | 270.4636   | 250.0000  | 108.2    |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 10.433 | 549244 | 314668    | 1.7455     | 408.2043   | 375.0000  | 108.9    |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 10.430 | 734101 | 313585    | 2.3410     | 547.4764   | 500.0000  | 109.5    |

# Quantitative Analysis Results Summary Report

**Compound: o-Xylene**

| Data File | Sample Type | ISTD             | RT     | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|--------|--------|-----------|------------|------------|-----------|----------|
| 04JAN23.D | QC          | Chlorobenzene-d5 | 10.430 | 174061 | 307868    | 0.5654     | 132.2214   | 125.0000  |          |

**Compound: Styrene**

| Data File | Sample Type | ISTD             | RT     | Resp    | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------|--------|---------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | Chlorobenzene-d5 |        |         | 301196    |            | ND         |           |          |
| 04JAN10.D | Calibration | Chlorobenzene-d5 | 10.444 | 4408    | 296081    | 0.0149     | 2.1625     | 2.5000    | 86.5     |
| 04JAN11.D | Calibration | Chlorobenzene-d5 | 10.449 | 23472   | 296554    | 0.0791     | 11.4968    | 12.5000   | 92.0     |
| 04JAN12.D | Calibration | Chlorobenzene-d5 | 10.447 | 48569   | 301338    | 0.1612     | 23.4119    | 25.0000   | 93.6     |
| 04JAN13.D | Calibration | Chlorobenzene-d5 | 10.444 | 96576   | 300356    | 0.3215     | 46.7052    | 50.0000   | 93.4     |
| 04JAN15.D | Calibration | Chlorobenzene-d5 | 10.447 | 268375  | 306491    | 0.8756     | 127.1910   | 125.0000  | 101.8    |
| 04JAN17.D | Calibration | Chlorobenzene-d5 | 10.446 | 605646  | 316399    | 1.9142     | 278.0455   | 250.0000  | 111.2    |
| 04JAN19.D | Calibration | Chlorobenzene-d5 | 10.447 | 896331  | 314668    | 2.8485     | 413.7595   | 375.0000  | 110.3    |
| 04JAN21.D | Calibration | Chlorobenzene-d5 | 10.449 | 1199879 | 313585    | 3.8263     | 555.7946   | 500.0000  | 111.2    |
| 04JAN23.D | QC          | Chlorobenzene-d5 | 10.449 | 291425  | 307868    | 0.9466     | 137.4974   | 125.0000  |          |

**Compound: Bromoform**

| Data File | Sample Type | ISTD                   | RT     | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------------|--------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | 1,4-Dichlorobenzene-d4 |        |        | 231562    |            | ND         |           |          |
| 04JAN10.D | Calibration | 1,4-Dichlorobenzene-d4 | 10.625 | 708    | 227879    | 0.0031     | 2.4287     | 2.5000    | 97.1     |
| 04JAN11.D | Calibration | 1,4-Dichlorobenzene-d4 | 10.625 | 3652   | 242142    | 0.0151     | 11.7860    | 12.5000   | 94.3     |
| 04JAN12.D | Calibration | 1,4-Dichlorobenzene-d4 | 10.625 | 7972   | 240335    | 0.0332     | 25.9212    | 25.0000   | 103.7    |
| 04JAN13.D | Calibration | 1,4-Dichlorobenzene-d4 | 10.625 | 16073  | 248636    | 0.0646     | 50.5170    | 50.0000   | 101.0    |
| 04JAN15.D | Calibration | 1,4-Dichlorobenzene-d4 | 10.628 | 39165  | 264477    | 0.1481     | 115.7218   | 125.0000  | 92.6     |
| 04JAN17.D | Calibration | 1,4-Dichlorobenzene-d4 | 10.628 | 87836  | 266553    | 0.3295     | 257.5099   | 250.0000  | 103.0    |
| 04JAN19.D | Calibration | 1,4-Dichlorobenzene-d4 | 10.628 | 129038 | 266611    | 0.4840     | 378.2200   | 375.0000  | 100.9    |
| 04JAN21.D | Calibration | 1,4-Dichlorobenzene-d4 | 10.625 | 175918 | 262971    | 0.6690     | 522.7660   | 500.0000  | 104.6    |
| 04JAN23.D | QC          | 1,4-Dichlorobenzene-d4 | 10.628 | 42560  | 255907    | 0.1663     | 129.9644   | 125.0000  |          |

**Compound: p-Bromofluorobenzene**

| Data File | Sample Type | ISTD                   | RT     | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------------|--------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | 1,4-Dichlorobenzene-d4 | 10.951 | 226743 | 231562    | 0.9792     | 267.2815   |           |          |
| 04JAN10.D | Calibration | 1,4-Dichlorobenzene-d4 | 10.951 | 2719   | 227879    | 0.0119     | 3.2569     | 2.5000    | 130.3    |
| 04JAN11.D | Calibration | 1,4-Dichlorobenzene-d4 | 10.948 | 10059  | 242142    | 0.0415     | 11.3393    | 12.5000   | 90.7     |
| 04JAN12.D | Calibration | 1,4-Dichlorobenzene-d4 | 10.951 | 22267  | 240335    | 0.0926     | 25.2899    | 25.0000   | 101.2    |
| 04JAN13.D | Calibration | 1,4-Dichlorobenzene-d4 | 10.951 | 42506  | 248636    | 0.1710     | 46.6647    | 50.0000   | 93.3     |
| 04JAN15.D | Calibration | 1,4-Dichlorobenzene-d4 | 10.954 | 114269 | 264477    | 0.4321     | 117.9350   | 125.0000  | 94.3     |
| 04JAN17.D | Calibration | 1,4-Dichlorobenzene-d4 | 10.951 | 261042 | 266553    | 0.9793     | 267.3186   | 250.0000  | 106.9    |
| 04JAN19.D | Calibration | 1,4-Dichlorobenzene-d4 | 10.951 | 385474 | 266611    | 1.4458     | 394.6566   | 375.0000  | 105.2    |
| 04JAN21.D | Calibration | 1,4-Dichlorobenzene-d4 | 10.949 | 521580 | 262971    | 1.9834     | 541.3964   | 500.0000  | 108.3    |
| 04JAN23.D | QC          | 1,4-Dichlorobenzene-d4 | 10.951 | 253034 | 255907    | 0.9888     | 269.8976   | 250.0000  |          |



# Quantitative Analysis Results Summary Report

**Compound: Bromobenzene**

| Data File | Sample Type | ISTD                   | RT     | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------------|--------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | 1,4-Dichlorobenzene-d4 |        |        | 231562    |            | ND         |           |          |
| 04JAN10.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.088 | 2024   | 227879    | 0.0089     | 2.7439     | 2.5000    | 109.8    |
| 04JAN11.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.096 | 9663   | 242142    | 0.0399     | 12.3310    | 12.5000   | 98.6     |
| 04JAN12.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.094 | 19259  | 240335    | 0.0801     | 24.7613    | 25.0000   | 99.0     |
| 04JAN13.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.093 | 38282  | 248636    | 0.1540     | 47.5759    | 50.0000   | 95.2     |
| 04JAN15.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.094 | 102265 | 264477    | 0.3867     | 119.4801   | 125.0000  | 95.6     |
| 04JAN17.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.093 | 227127 | 266553    | 0.8521     | 263.2944   | 250.0000  | 105.3    |
| 04JAN19.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.093 | 333431 | 266611    | 1.2506     | 386.4420   | 375.0000  | 103.1    |
| 04JAN21.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.094 | 439147 | 262971    | 1.6699     | 516.0104   | 500.0000  | 103.2    |
| 04JAN23.D | QC          | 1,4-Dichlorobenzene-d4 | 11.093 | 109054 | 255907    | 0.4261     | 131.6788   | 125.0000  |          |

**Compound: 1,1,2,2-Tetrachloroethane**

| Data File | Sample Type | ISTD                   | RT     | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------------|--------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | 1,4-Dichlorobenzene-d4 |        |        | 231562    |            | ND         |           |          |
| 04JAN10.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.113 | 1142   | 227879    | 0.0050     | 2.6916     | 2.5000    | 107.7    |
| 04JAN11.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.116 | 5793   | 242142    | 0.0239     | 12.8437    | 12.5000   | 102.7    |
| 04JAN12.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.110 | 12440  | 240335    | 0.0518     | 27.7883    | 25.0000   | 111.2    |
| 04JAN13.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.105 | 22514  | 248636    | 0.0906     | 48.6124    | 50.0000   | 97.2     |
| 04JAN15.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.116 | 56958  | 264477    | 0.2154     | 115.6179   | 125.0000  | 92.5     |
| 04JAN17.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.113 | 124205 | 266553    | 0.4660     | 250.1577   | 250.0000  | 100.1    |
| 04JAN19.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.110 | 182470 | 266611    | 0.6844     | 367.4276   | 375.0000  | 98.0     |
| 04JAN21.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.113 | 240837 | 262971    | 0.9158     | 491.6700   | 500.0000  | 98.3     |
| 04JAN23.D | QC          | 1,4-Dichlorobenzene-d4 | 11.113 | 60763  | 255907    | 0.2374     | 127.4722   | 125.0000  |          |

**Compound: 1,2,3-Trichloropropane**

| Data File | Sample Type | ISTD                   | RT     | Resp  | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------------|--------|-------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | 1,4-Dichlorobenzene-d4 |        |       | 231562    |            | ND         |           |          |
| 04JAN10.D | Calibration | 1,4-Dichlorobenzene-d4 |        |       | 227879    |            | ND         | 2.5000    |          |
| 04JAN11.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.144 | 1654  | 242142    | 0.0068     | 13.7084    | 12.5000   | 109.7    |
| 04JAN12.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.149 | 3200  | 240335    | 0.0133     | 26.7144    | 25.0000   | 106.9    |
| 04JAN13.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.146 | 6096  | 248636    | 0.0245     | 49.1924    | 50.0000   | 98.4     |
| 04JAN15.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.147 | 14846 | 264477    | 0.0561     | 112.6261   | 125.0000  | 90.1     |
| 04JAN17.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.152 | 33115 | 266553    | 0.1242     | 249.2635   | 250.0000  | 99.7     |
| 04JAN19.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.149 | 48325 | 266611    | 0.1813     | 363.6732   | 375.0000  | 97.0     |
| 04JAN21.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.146 | 64422 | 262971    | 0.2450     | 491.5229   | 500.0000  | 98.3     |
| 04JAN23.D | QC          | 1,4-Dichlorobenzene-d4 | 11.146 | 15682 | 255907    | 0.0613     | 122.9523   | 125.0000  |          |

**Compound: 2-Chlorotoluene**

| Data File | Sample Type | ISTD                   | RT     | Resp | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------------|--------|------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | 1,4-Dichlorobenzene-d4 |        |      | 231562    |            | ND         |           |          |
| 04JAN10.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.292 | 1844 | 227879    | 0.0081     | 2.5124     | 2.5000    | 100.5    |
| 04JAN11.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.289 | 8731 | 242142    | 0.0361     | 11.1977    | 12.5000   | 89.6     |

# Quantitative Analysis Results Summary Report

## Compound: 2-Chlorotoluene

| Data File | Sample Type | ISTD                   | RT     | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------------|--------|--------|-----------|------------|------------|-----------|----------|
| 04JAN12.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.286 | 19390  | 240335    | 0.0807     | 25.0550    | 25.0000   | 100.2    |
| 04JAN13.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.289 | 37987  | 248636    | 0.1528     | 47.4466    | 50.0000   | 94.9     |
| 04JAN15.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.292 | 102424 | 264477    | 0.3873     | 120.2675   | 125.0000  | 96.2     |
| 04JAN17.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.291 | 229396 | 266553    | 0.8606     | 267.2616   | 250.0000  | 106.9    |
| 04JAN19.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.291 | 336386 | 266611    | 1.2617     | 391.8269   | 375.0000  | 104.5    |
| 04JAN21.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.292 | 455991 | 262971    | 1.7340     | 538.4964   | 500.0000  | 107.7    |
| 04JAN23.D | QC          | 1,4-Dichlorobenzene-d4 | 11.291 | 108192 | 255907    | 0.4228     | 131.2948   | 125.0000  |          |

## Compound: 4-Chlorotoluene

| Data File | Sample Type | ISTD                   | RT     | Resp    | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------------|--------|---------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | 1,4-Dichlorobenzene-d4 |        |         | 231562    |            | ND         |           |          |
| 04JAN10.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.400 | 5419    | 227879    | 0.0238     | 2.2650     | 2.5000    | 90.6     |
| 04JAN11.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.400 | 28532   | 242142    | 0.1178     | 11.2233    | 12.5000   | 89.8     |
| 04JAN12.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.400 | 61551   | 240335    | 0.2561     | 24.3936    | 25.0000   | 97.6     |
| 04JAN13.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.400 | 126308  | 248636    | 0.5080     | 48.3865    | 50.0000   | 96.8     |
| 04JAN15.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.400 | 336146  | 264477    | 1.2710     | 121.0591   | 125.0000  | 96.8     |
| 04JAN17.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.400 | 748435  | 266553    | 2.8078     | 267.4409   | 250.0000  | 107.0    |
| 04JAN19.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.400 | 1109221 | 266611    | 4.1604     | 396.2756   | 375.0000  | 105.7    |
| 04JAN21.D | Calibration | 1,4-Dichlorobenzene-d4 | 11.400 | 1468376 | 262971    | 5.5838     | 531.8471   | 500.0000  | 106.4    |
| 04JAN23.D | QC          | 1,4-Dichlorobenzene-d4 | 11.400 | 368295  | 255907    | 1.4392     | 137.0790   | 125.0000  |          |

## Compound: 1,3-Dichlorobenzene

| Data File | Sample Type | ISTD                   | RT     | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------------|--------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | 1,4-Dichlorobenzene-d4 |        |        | 231562    |            | ND         |           |          |
| 04JAN10.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.033 | 3541   | 227879    | 0.0155     | 2.6327     | 2.5000    | 105.3    |
| 04JAN11.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.036 | 16932  | 242142    | 0.0699     | 11.8473    | 12.5000   | 94.8     |
| 04JAN12.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.033 | 36559  | 240335    | 0.1521     | 25.7725    | 25.0000   | 103.1    |
| 04JAN13.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.033 | 69539  | 248636    | 0.2797     | 47.3853    | 50.0000   | 94.8     |
| 04JAN15.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.031 | 183404 | 264477    | 0.6935     | 117.4899   | 125.0000  | 94.0     |
| 04JAN17.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.033 | 406895 | 266553    | 1.5265     | 258.6297   | 250.0000  | 103.5    |
| 04JAN19.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.033 | 603674 | 266611    | 2.2643     | 383.6225   | 375.0000  | 102.3    |
| 04JAN21.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.033 | 793993 | 262971    | 3.0193     | 511.5504   | 500.0000  | 102.3    |
| 04JAN23.D | QC          | 1,4-Dichlorobenzene-d4 | 12.033 | 204088 | 255907    | 0.7975     | 135.1185   | 125.0000  |          |

## Compound: 1,4-Dichlorobenzene

| Data File | Sample Type | ISTD                   | RT     | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------------|--------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | 1,4-Dichlorobenzene-d4 |        |        | 231562    |            | ND         |           |          |
| 04JAN10.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.125 | 3787   | 227879    | 0.0166     | 2.7613     | 2.5000    | 110.5    |
| 04JAN11.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.122 | 17438  | 242142    | 0.0720     | 11.9662    | 12.5000   | 95.7     |
| 04JAN12.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.125 | 36635  | 240335    | 0.1524     | 25.3284    | 25.0000   | 101.3    |
| 04JAN13.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.125 | 71841  | 248636    | 0.2889     | 48.0106    | 50.0000   | 96.0     |
| 04JAN15.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.125 | 189045 | 264477    | 0.7148     | 118.7699   | 125.0000  | 95.0     |

# Quantitative Analysis Results Summary Report

**Compound: 1,4-Dichlorobenzene**

| Data File | Sample Type | ISTD                   | RT     | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------------|--------|--------|-----------|------------|------------|-----------|----------|
| 04JAN17.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.122 | 408934 | 266553    | 1.5342     | 254.9170   | 250.0000  | 102.0    |
| 04JAN19.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.125 | 595919 | 266611    | 2.2352     | 371.3969   | 375.0000  | 99.0     |
| 04JAN21.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.125 | 794954 | 262971    | 3.0230     | 502.3001   | 500.0000  | 100.5    |
| 04JAN23.D | QC          | 1,4-Dichlorobenzene-d4 | 12.122 | 200032 | 255907    | 0.7817     | 129.8812   | 125.0000  |          |

**Compound: 1,2-Dichlorobenzene**

| Data File | Sample Type | ISTD                   | RT     | Resp   | ISTD Resp | Resp Ratio | Final Conc | Exp. Conc | Accuracy |
|-----------|-------------|------------------------|--------|--------|-----------|------------|------------|-----------|----------|
| 04JAN09.D | Blank       | 1,4-Dichlorobenzene-d4 |        |        | 231562    |            | ND         |           |          |
| 04JAN10.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.499 | 3104   | 227879    | 0.0136     | 2.7307     | 2.5000    | 109.2    |
| 04JAN11.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.493 | 14666  | 242142    | 0.0606     | 12.1423    | 12.5000   | 97.1     |
| 04JAN12.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.488 | 29899  | 240335    | 0.1244     | 24.9402    | 25.0000   | 99.8     |
| 04JAN13.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.491 | 60213  | 248636    | 0.2422     | 48.5498    | 50.0000   | 97.1     |
| 04JAN15.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.493 | 152284 | 264477    | 0.5758     | 115.4323   | 125.0000  | 92.3     |
| 04JAN17.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.493 | 342576 | 266553    | 1.2852     | 257.6524   | 250.0000  | 103.1    |
| 04JAN19.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.493 | 499147 | 266611    | 1.8722     | 375.3283   | 375.0000  | 100.1    |
| 04JAN21.D | Calibration | 1,4-Dichlorobenzene-d4 | 12.493 | 664247 | 262971    | 2.5259     | 506.3871   | 500.0000  | 101.3    |
| 04JAN23.D | QC          | 1,4-Dichlorobenzene-d4 | 12.493 | 164299 | 255907    | 0.6420     | 128.7104   | 125.0000  |          |

# Initial Calibration Report - VOA5975C

Method Path            \\MASSHUNTER\Org\Data\Methods\Quant\VOA5975C\VOA5975C\_010422\_CAL  
 Method File            VOA5975C\_8260B\_SHT\_DoD\_L4\_010422.m  
 Batch Name             D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422\_8260B.batch.bin  
 Last Calib Update     1/9/2022 8:59:52 PM

| Level Name | Calibration Files                       | Acq. Date-Time      | Level Last Update Time |
|------------|-----------------------------------------|---------------------|------------------------|
| 1          | D:\Org\Data\VOA5975C\VG010422\04JAN10.D | 1/4/2022 3:33:04 PM | 1/5/2022 11:05:51 AM   |
| 2          | D:\Org\Data\VOA5975C\VG010422\04JAN11.D | 1/4/2022 4:00:35 PM | 1/5/2022 11:05:51 AM   |
| 3          | D:\Org\Data\VOA5975C\VG010422\04JAN12.D | 1/4/2022 4:28:05 PM | 1/5/2022 11:05:51 AM   |
| 4          | D:\Org\Data\VOA5975C\VG010422\04JAN13.D | 1/4/2022 4:55:32 PM | 1/5/2022 11:05:51 AM   |
| 5          | D:\Org\Data\VOA5975C\VG010422\04JAN15.D | 1/4/2022 5:50:25 PM | 1/5/2022 11:05:51 AM   |
| 6          | D:\Org\Data\VOA5975C\VG010422\04JAN17.D | 1/4/2022 6:45:10 PM | 1/5/2022 11:05:51 AM   |
| 7          | D:\Org\Data\VOA5975C\VG010422\04JAN19.D | 1/4/2022 7:39:45 PM | 1/5/2022 11:05:51 AM   |
| 8          | D:\Org\Data\VOA5975C\VG010422\04JAN21.D | 1/4/2022 8:34:31 PM | 1/5/2022 11:05:51 AM   |

| Compound                         | Curve Fit | 1      | 2      | 3      | 4      | 5      | 6      | 7      | 8      | Avg RF   | %RSD   |
|----------------------------------|-----------|--------|--------|--------|--------|--------|--------|--------|--------|----------|--------|
| ----- ISTD -----                 |           |        |        |        |        |        |        |        |        |          |        |
| I Fluorobenzene                  |           |        |        |        |        |        |        |        |        |          |        |
| T Dichlorodifluoromethane        | Avg RF    |        | 0.3162 | 0.3365 | 0.3242 | 0.3350 | 0.3304 | 0.3267 | 0.3242 | 0.3276   | 2.141  |
| T Chloromethane                  | Avg RF    |        | 0.4411 | 0.4190 | 0.3960 | 0.3901 | 0.3821 | 0.3733 | 0.3819 | 0.3976   | 6.061  |
| T Vinyl chloride                 | Avg RF    |        | 0.3591 | 0.3671 | 0.3503 | 0.3603 | 0.3559 | 0.3553 | 0.3566 | 0.3578   | 1.449  |
| T Bromomethane                   | Avg RF    |        | 0.1542 | 0.1650 | 0.1523 | 0.1583 | 0.1611 | 0.1643 | 0.1648 | 0.1600   | 3.267  |
| T Chloroethane                   | Avg RF    |        | 0.2107 | 0.1851 | 0.1638 | 0.1735 | 0.1642 | 0.1721 | 0.1706 | 0.1771   | 9.265  |
| T Trichlorofluoromethane         | Avg RF    |        | 0.4037 | 0.4735 | 0.4380 | 0.4586 | 0.4602 | 0.4399 | 0.4349 | 0.4441   | 5.118  |
| T 1,1-Dichloroethene             | Avg RF    |        | 0.2399 | 0.2607 | 0.2458 | 0.2415 | 0.2600 | 0.2554 | 0.2594 | 0.2518   | 3.629  |
| T Methylene chloride             | Avg RF    |        | 0.4640 | 0.3906 | 0.3745 | 0.3285 | 0.3496 | 0.3446 | 0.3467 | 0.3712   | 12.340 |
| T trans-1,2-Dichloroethene       | Avg RF    |        | 0.2570 | 0.2617 | 0.2544 | 0.2439 | 0.2617 | 0.2577 | 0.2621 | 0.2569   | 2.508  |
| T Methyl tert-butyl ether (MTBE) | Avg RF    |        | 0.3274 | 0.3061 | 0.3157 | 0.3378 | 0.3440 | 0.3464 | 0.3472 | 0.3321   | 4.880  |
| T 1,1-Dichloroethane             | Avg RF    |        | 0.4616 | 0.4913 | 0.4704 | 0.4519 | 0.4943 | 0.4852 | 0.4929 | 0.4782   | 3.547  |
| T 2,2-Dichloropropane            | Avg RF    |        | 0.3578 | 0.3765 | 0.3611 | 0.3392 | 0.3627 | 0.3534 | 0.3576 | 0.3583   | 3.118  |
| T cis-1,2-Dichloroethene         | Avg RF    |        | 0.2618 | 0.2559 | 0.2522 | 0.2430 | 0.2728 | 0.2686 | 0.2688 | 0.2605   | 4.101  |
| T Methyl ethyl ketone            | Avg RF    |        | 0.0344 | 0.0332 | 0.0338 | 0.0327 | 0.0379 | 0.0373 | 0.0376 | 0.0353 # | 6.353  |
| T Bromochloromethane             | Avg RF    |        | 0.1118 | 0.1098 | 0.1114 | 0.1019 | 0.1066 | 0.1070 | 0.1067 | 0.1079   | 3.188  |
| T Chloroform                     | Avg RF    | 0.5510 | 0.4975 | 0.4602 | 0.4588 | 0.4363 | 0.4723 | 0.4657 | 0.4656 | 0.4759   | 7.299  |
| T 1,1,1-Trichloroethane          | Avg RF    |        | 0.4349 | 0.4492 | 0.4306 | 0.4231 | 0.4616 | 0.4599 | 0.4628 | 0.4460   | 3.677  |
| S Dibromofluoromethane           | Avg RF    |        | 0.2374 | 0.2414 | 0.2269 | 0.2169 | 0.2440 | 0.2416 | 0.2404 | 0.2355   | 4.222  |
| T Carbon tetrachloride           | Avg RF    |        | 0.4308 | 0.4355 | 0.4197 | 0.4200 | 0.4586 | 0.4534 | 0.4581 | 0.4394   | 3.906  |
| T 1,1-Dichloropropene            | Avg RF    |        | 0.3440 | 0.3695 | 0.3623 | 0.3635 | 0.4015 | 0.4016 | 0.4122 | 0.3792   | 6.770  |
| S 1,2-Dichloroethane-d4          | Avg RF    |        | 0.1030 | 0.1047 | 0.0979 | 0.0949 | 0.1051 | 0.1026 | 0.1038 | 0.1017   | 3.759  |
| T Benzene                        | Avg RF    | 1.0907 | 0.9699 | 0.9473 | 0.9557 | 0.9313 | 1.0254 | 1.0242 | 1.0186 | 0.9954   | 5.369  |
| T 1,2-Dichloroethane             | Avg RF    | 0.3133 | 0.2669 | 0.2527 | 0.2638 | 0.2547 | 0.2714 | 0.2635 | 0.2679 | 0.2693   | 7.024  |
| ----- ISTD -----                 |           |        |        |        |        |        |        |        |        |          |        |
| I Chlorobenzene-d5               |           |        |        |        |        |        |        |        |        |          |        |
| T Trichloroethene                | Avg RF    |        | 0.7042 | 0.7283 | 0.7105 | 0.7447 | 0.7910 | 0.7932 | 0.8058 | 0.7540   | 5.603  |
| T 1,2-Dichloropropane            | Avg RF    |        | 0.6399 | 0.6663 | 0.6304 | 0.6472 | 0.6757 | 0.6877 | 0.6953 | 0.6632   | 3.729  |
| T Dibromomethane                 | Avg RF    |        | 0.3153 | 0.2673 | 0.2662 | 0.2651 | 0.2828 | 0.2845 | 0.2807 | 0.2803   | 6.261  |
| T Bromodichloromethane           | Avg RF    |        | 0.7798 | 0.7547 | 0.7308 | 0.7548 | 0.7958 | 0.7966 | 0.8019 | 0.7735   | 3.503  |

## Initial Calibration Report - VOA5975C

| Compound                    | Curve Fit | 1      | 2      | 3      | 4      | 5      | 6      | 7      | 8      | Avg RF | %RSD  |
|-----------------------------|-----------|--------|--------|--------|--------|--------|--------|--------|--------|--------|-------|
| T cis-1,3-Dichloropropene   | Avg RF    |        | 0.8447 | 0.8134 | 0.8138 | 0.8445 | 0.9280 | 0.9347 | 0.9426 | 0.8745 | 6.654 |
| S Toluene-d8                | Avg RF    |        | 2.1796 | 2.2458 | 2.2715 | 2.3373 | 2.6021 | 2.6054 | 2.6222 | 2.4091 | 8.032 |
| T Toluene                   | Avg RF    | 1.7019 | 1.4698 | 1.5383 | 1.5301 | 1.5969 | 1.7129 | 1.7229 | 1.7462 | 1.6274 | 6.538 |
| T trans-1,3-Dichloropropene | Avg RF    |        | 0.5856 | 0.5924 | 0.5856 | 0.6050 | 0.6569 | 0.6675 | 0.6645 | 0.6225 | 6.190 |
| T 1,1,2-Trichloroethane     | Avg RF    |        | 0.3433 | 0.3351 | 0.3144 | 0.3046 | 0.3220 | 0.3227 | 0.3276 | 0.3242 | 3.951 |
| T Tetrachloroethene         | Avg RF    | 0.7110 | 0.6230 | 0.6744 | 0.6147 | 0.6368 | 0.6898 | 0.6779 | 0.6837 | 0.6639 | 5.221 |
| T 1,3-Dichloropropane       | Avg RF    |        | 0.6047 | 0.6221 | 0.6235 | 0.6276 | 0.6722 | 0.6622 | 0.6521 | 0.6378 | 3.855 |
| T Chlorodibromomethane      | Avg RF    |        | 0.5205 | 0.4936 | 0.4687 | 0.4895 | 0.5237 | 0.5239 | 0.5275 | 0.5068 | 4.501 |
| T 1,2-Dibromoethane         | Avg RF    |        | 0.3649 | 0.3455 | 0.3502 | 0.3382 | 0.3657 | 0.3572 | 0.3602 | 0.3545 | 2.909 |
| T Chlorobenzene             | Avg RF    |        | 1.7846 | 1.7604 | 1.6889 | 1.7202 | 1.8405 | 1.8384 | 1.8387 | 1.7817 | 3.458 |
| T 1,1,1,2-Tetrachloroethane | Avg RF    |        | 0.6389 | 0.6016 | 0.5917 | 0.5932 | 0.6348 | 0.6513 | 0.6481 | 0.6228 | 4.223 |
| T Ethylbenzene              | Avg RF    | 3.1353 | 2.7294 | 2.9345 | 2.8927 | 3.0288 | 3.2979 | 3.3352 | 3.3662 | 3.0900 | 7.526 |
| T m+p-Xylenes               | Avg RF    | 1.2179 | 1.0635 | 1.0995 | 1.1112 | 1.2021 | 1.3051 | 1.3014 | 1.3058 | 1.2008 | 8.296 |
| T o-Xylene                  | Avg RF    |        | 0.9117 | 1.0109 | 1.0157 | 1.0539 | 1.1565 | 1.1636 | 1.1705 | 1.0690 | 9.204 |
| T Styrene                   | Avg RF    | 1.4888 | 1.5830 | 1.6118 | 1.6077 | 1.7513 | 1.9142 | 1.8990 | 1.9132 | 1.7211 | 9.933 |
| I 1,4-Dichlorobenzene-d4    |           |        |        |        |        |        |        |        |        |        |       |
| ----- ISTD -----            |           |        |        |        |        |        |        |        |        |        |       |
| T Bromoform                 | Avg RF    |        | 0.3016 | 0.3317 | 0.3232 | 0.2962 | 0.3295 | 0.3227 | 0.3345 | 0.3199 | 4.706 |
| S p-Bromofluorobenzene      | Avg RF    |        | 0.8308 | 0.9265 | 0.8548 | 0.8641 | 0.9793 | 0.9639 | 0.9917 | 0.9159 | 7.165 |
| T Bromobenzene              | Avg RF    |        | 0.7981 | 0.8013 | 0.7698 | 0.7733 | 0.8521 | 0.8338 | 0.8350 | 0.8091 | 3.949 |
| T 1,1,2,2-Tetrachloroethane | Avg RF    |        | 0.4785 | 0.5176 | 0.4528 | 0.4307 | 0.4660 | 0.4563 | 0.4579 | 0.4657 | 5.814 |
| T 1,2,3-Trichloropropane    | Avg RF    |        | 0.1366 | 0.1331 | 0.1226 | 0.1123 | 0.1242 | 0.1208 | 0.1225 | 0.1246 | 6.496 |
| T 2-Chlorotoluene           | Avg RF    |        | 0.7211 | 0.8068 | 0.7639 | 0.7745 | 0.8606 | 0.8411 | 0.8670 | 0.8050 | 6.783 |
| T 4-Chlorotoluene           | Avg RF    |        | 2.3566 | 2.5611 | 2.5400 | 2.5420 | 2.8078 | 2.7736 | 2.7919 | 2.6247 | 6.481 |
| T 1,3-Dichlorobenzene       | Avg RF    | 1.5539 | 1.3985 | 1.5212 | 1.3984 | 1.3869 | 1.5265 | 1.5095 | 1.5097 | 1.4756 | 4.644 |
| T 1,4-Dichlorobenzene       | Avg RF    | 1.6618 | 1.4403 | 1.5243 | 1.4447 | 1.4296 | 1.5342 | 1.4901 | 1.5115 | 1.5046 | 4.999 |
| T 1,2-Dichlorobenzene       | Avg RF    | 1.3621 | 1.2114 | 1.2441 | 1.2109 | 1.1516 | 1.2852 | 1.2481 | 1.2630 | 1.2470 | 4.949 |


(RedFont and #) = Outlier Flag; (I) = Internal Standard; (T) = Target; (S) = Surrogate; (M) = Matrix Spike

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:39 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**Dichlorodifluoromethane %RSE = 2.1**

Dichlorodifluoromethane - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs

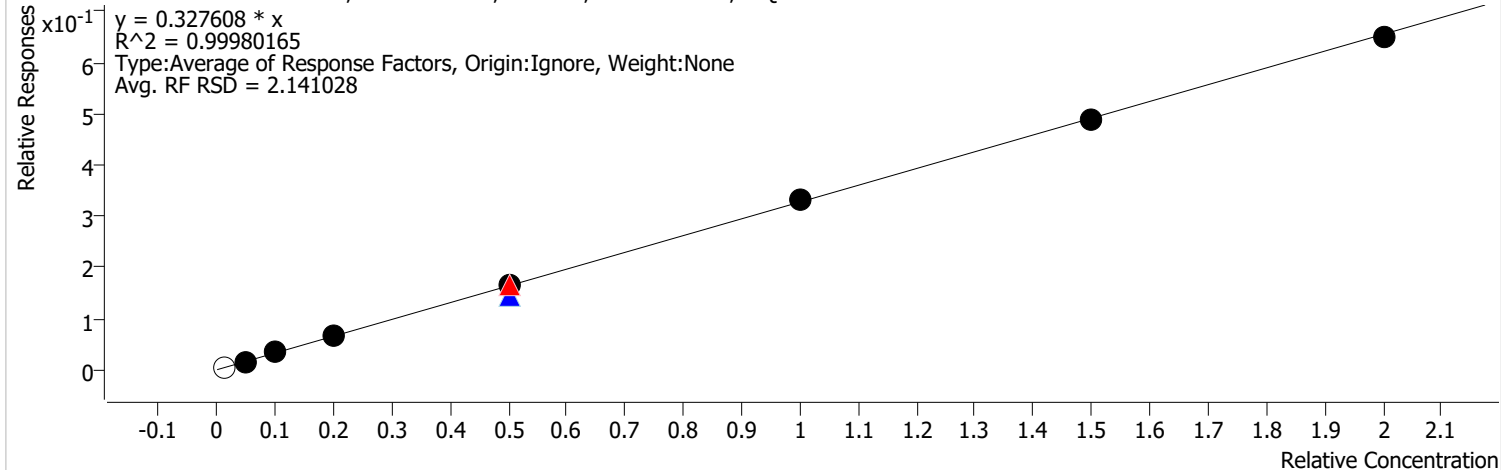


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 4353   | 2.5000    | 0.5647       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 12087  | 12.5000   | 0.3162       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 26627  | 25.0000   | 0.3365       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 50457  | 50.0000   | 0.3242       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 116936 | 125.0000  | 0.2919       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 137933 | 125.0000  | 0.3350       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 137933 | 125.0000  | 0.3350       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 276334 | 250.0000  | 0.3304       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 412544 | 375.0000  | 0.3267       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 545484 | 500.0000  | 0.3242       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:42 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**Chloromethane %RSE = 6.1**

Chloromethane - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs

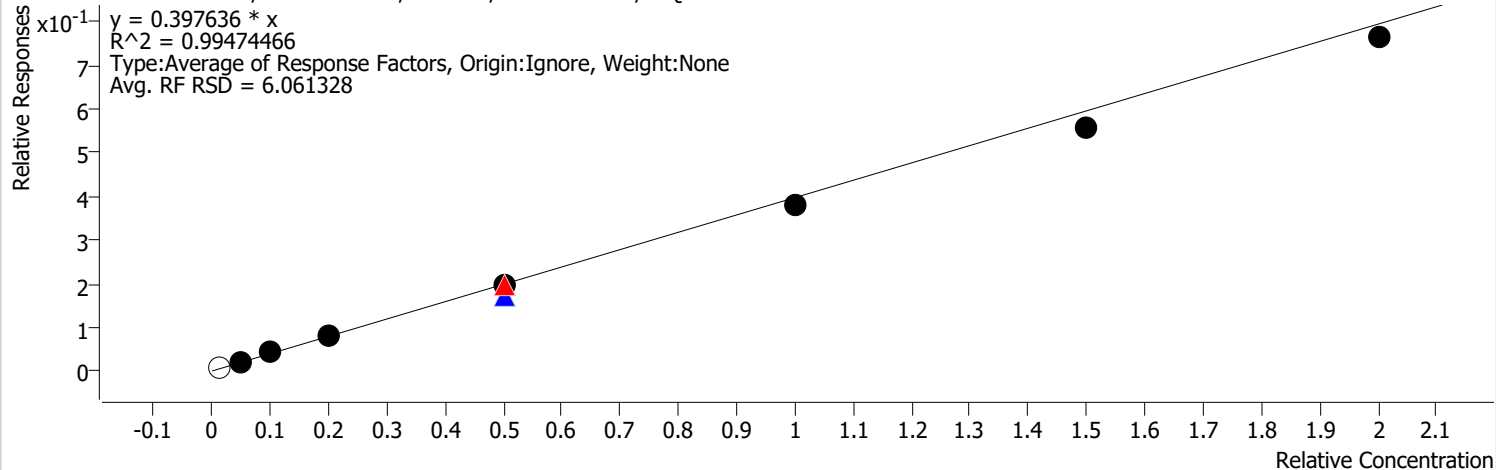


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 7435   | 2.5000    | 0.9645       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 16859  | 12.5000   | 0.4411       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 33153  | 25.0000   | 0.4190       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 61632  | 50.0000   | 0.3960       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 138617 | 125.0000  | 0.3460       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 160604 | 125.0000  | 0.3901       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 160604 | 125.0000  | 0.3901       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 319523 | 250.0000  | 0.3821       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 471454 | 375.0000  | 0.3733       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 642582 | 500.0000  | 0.3819       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:42 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**Vinyl chloride %RSE = 1.4**

Vinyl chloride - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs

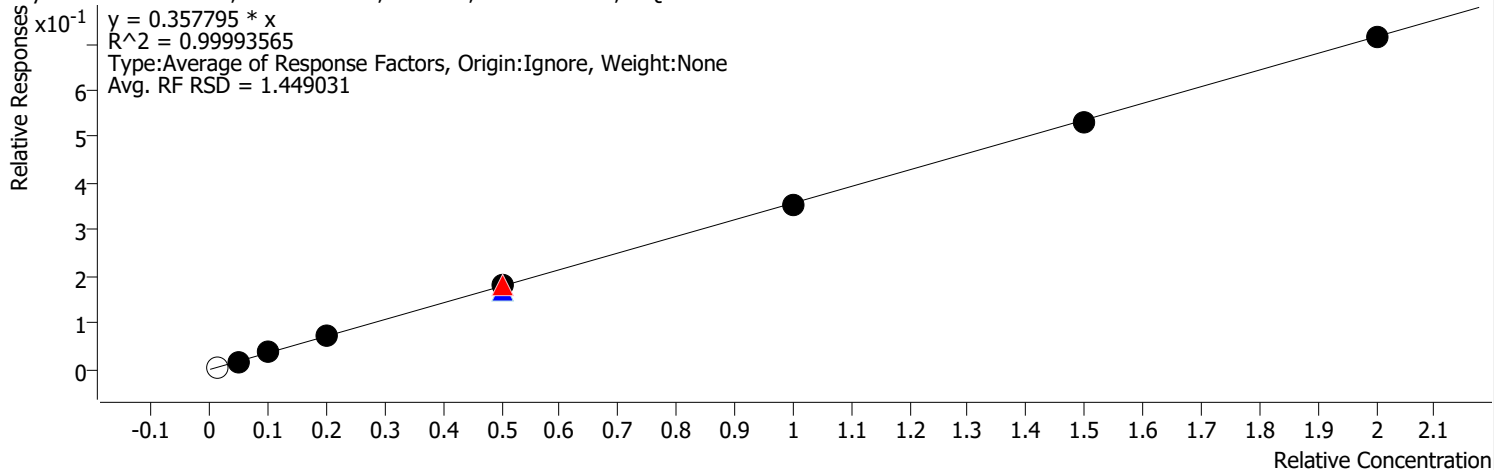

| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 4274   | 2.5000    | 0.5544       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 13724  | 12.5000   | 0.3591       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 29046  | 25.0000   | 0.3671       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 54521  | 50.0000   | 0.3503       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 137775 | 125.0000  | 0.3439       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 148358 | 125.0000  | 0.3603       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 148358 | 125.0000  | 0.3603       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 297604 | 250.0000  | 0.3559       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 448643 | 375.0000  | 0.3553       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 600092 | 500.0000  | 0.3566       |           |




# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:42 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**Bromomethane %RSE = 3.3**

Bromomethane - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs




| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 1902   | 2.5000    | 0.2467       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 5893   | 12.5000   | 0.1542       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 13054  | 25.0000   | 0.1650       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 23699  | 50.0000   | 0.1523       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 59947  | 125.0000  | 0.1496       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 65163  | 125.0000  | 0.1583       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 65163  | 125.0000  | 0.1583       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 134737 | 250.0000  | 0.1611       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 207491 | 375.0000  | 0.1643       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 277301 | 500.0000  | 0.1648       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:42 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**Chloroethane %RSE = 9.3**

Chloroethane - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs

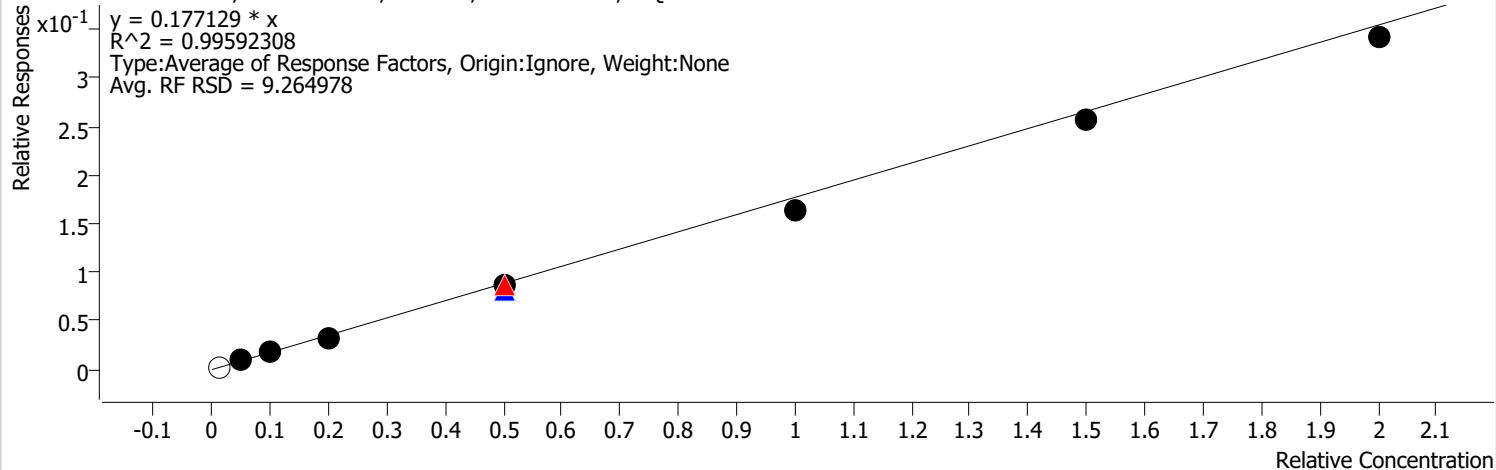


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 2178   | 2.5000    | 0.2825       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 8052   | 12.5000   | 0.2107       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 14646  | 25.0000   | 0.1851       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 25484  | 50.0000   | 0.1638       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 65619  | 125.0000  | 0.1638       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 71420  | 125.0000  | 0.1735       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 71420  | 125.0000  | 0.1735       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 137312 | 250.0000  | 0.1642       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 217393 | 375.0000  | 0.1721       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 287041 | 500.0000  | 0.1706       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:43 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**Trichlorofluoromethane %RSE = 5.1**

Trichlorofluoromethane - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs

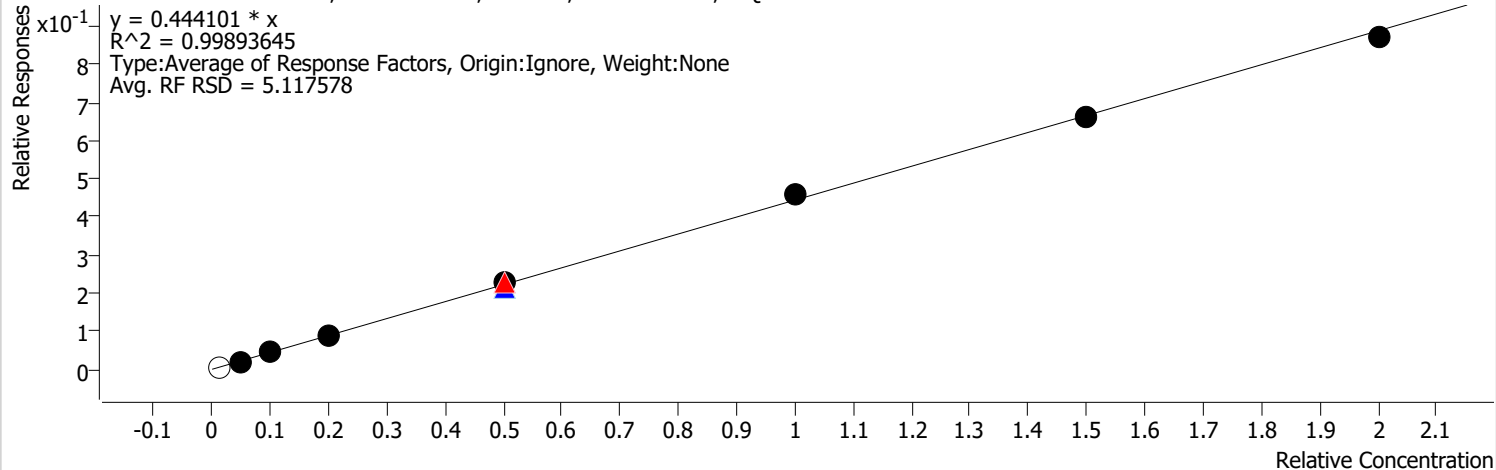


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 5030   | 2.5000    | 0.6525       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 15431  | 12.5000   | 0.4037       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 37464  | 25.0000   | 0.4735       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 68163  | 50.0000   | 0.4380       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 173333 | 125.0000  | 0.4327       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 188808 | 125.0000  | 0.4586       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 188808 | 125.0000  | 0.4586       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 384837 | 250.0000  | 0.4602       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 555477 | 375.0000  | 0.4399       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 731829 | 500.0000  | 0.4349       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:43 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**1,1-Dichloroethene %RSE = 3.6**

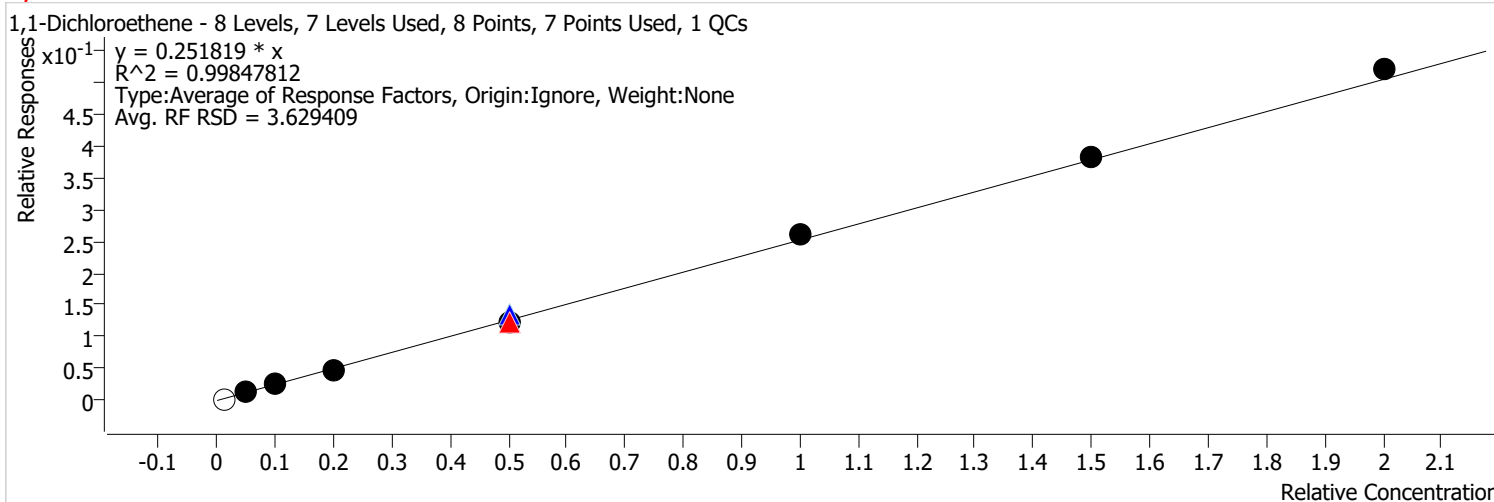


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 2084   | 2.5000    | 0.2703       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 9169   | 12.5000   | 0.2399       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 20631  | 25.0000   | 0.2607       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 38253  | 50.0000   | 0.2458       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 108512 | 125.0000  | 0.2709       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 99438  | 125.0000  | 0.2415       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 99438  | 125.0000  | 0.2415       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 217406 | 250.0000  | 0.2600       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 322557 | 375.0000  | 0.2554       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 436507 | 500.0000  | 0.2594       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:43 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**Methylene chloride %RSE = 12.3**

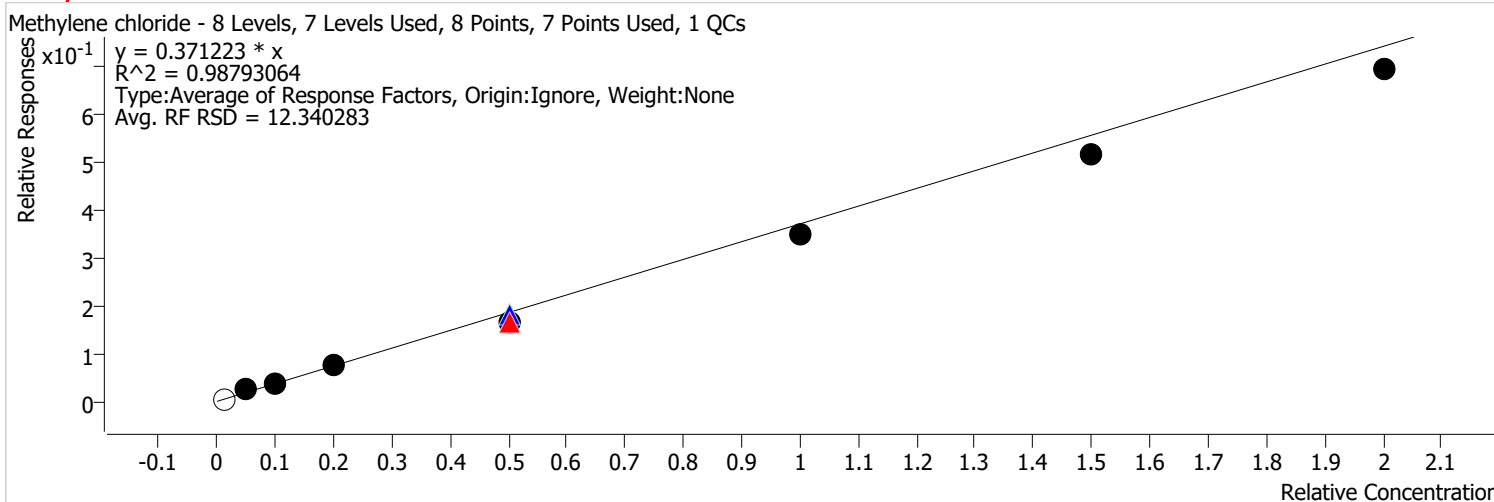


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 4095   | 2.5000    | 0.5312       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 17734  | 12.5000   | 0.4640       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 30908  | 25.0000   | 0.3906       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 58282  | 50.0000   | 0.3745       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 144585 | 125.0000  | 0.3609       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 135271 | 125.0000  | 0.3285       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 135271 | 125.0000  | 0.3285       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 292397 | 250.0000  | 0.3496       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 435116 | 375.0000  | 0.3446       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 583438 | 500.0000  | 0.3467       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:43 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**trans-1,2-Dichloroethene %RSE = 2.5**




| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 2146   | 2.5000    | 0.2784       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 9821   | 12.5000   | 0.2570       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 20706  | 25.0000   | 0.2617       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 39596  | 50.0000   | 0.2544       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 110909 | 125.0000  | 0.2769       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 100409 | 125.0000  | 0.2439       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 100409 | 125.0000  | 0.2439       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 218855 | 250.0000  | 0.2617       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 325415 | 375.0000  | 0.2577       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 440967 | 500.0000  | 0.2621       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:43 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**Methyl tert-butyl ether (MTBE) %RSE = 4.9**

Methyl tert-butyl ether (MTBE) - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs

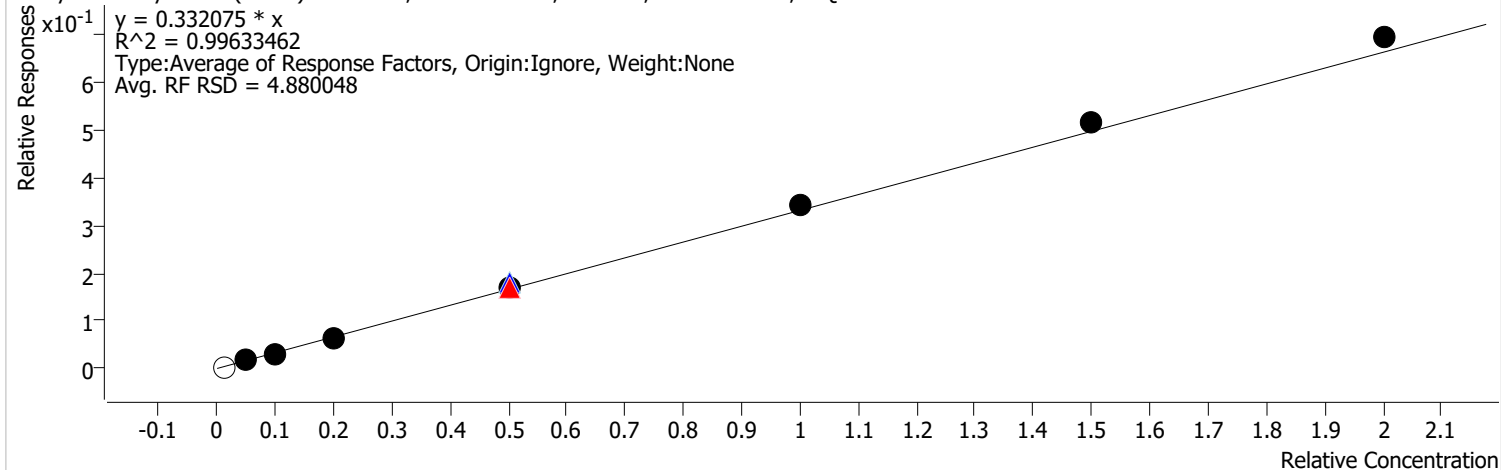


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 2717   | 2.5000    | 0.3524       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 12515  | 12.5000   | 0.3274       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 24218  | 25.0000   | 0.3061       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 49126  | 50.0000   | 0.3157       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 143378 | 125.0000  | 0.3579       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 139068 | 125.0000  | 0.3378       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 139068 | 125.0000  | 0.3378       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 287653 | 250.0000  | 0.3440       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 437439 | 375.0000  | 0.3464       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 584294 | 500.0000  | 0.3472       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:43 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**1,1-Dichloroethane %RSE = 3.5**

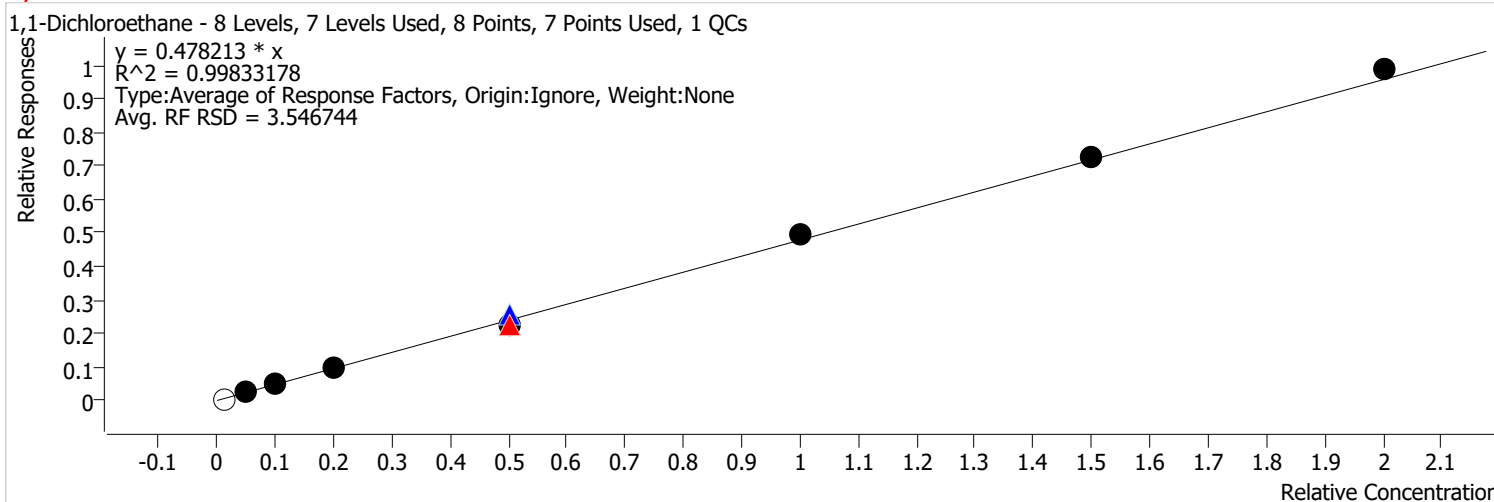

| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 3892   | 2.5000    | 0.5049       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 17642  | 12.5000   | 0.4616       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 38874  | 25.0000   | 0.4913       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 73205  | 50.0000   | 0.4704       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 208131 | 125.0000  | 0.5195       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 186052 | 125.0000  | 0.4519       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 186052 | 125.0000  | 0.4519       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 413408 | 250.0000  | 0.4943       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 612660 | 375.0000  | 0.4852       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 829359 | 500.0000  | 0.4929       |           |




# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:43 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**2,2-Dichloropropane %RSE = 3.1**

2,2-Dichloropropane - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs

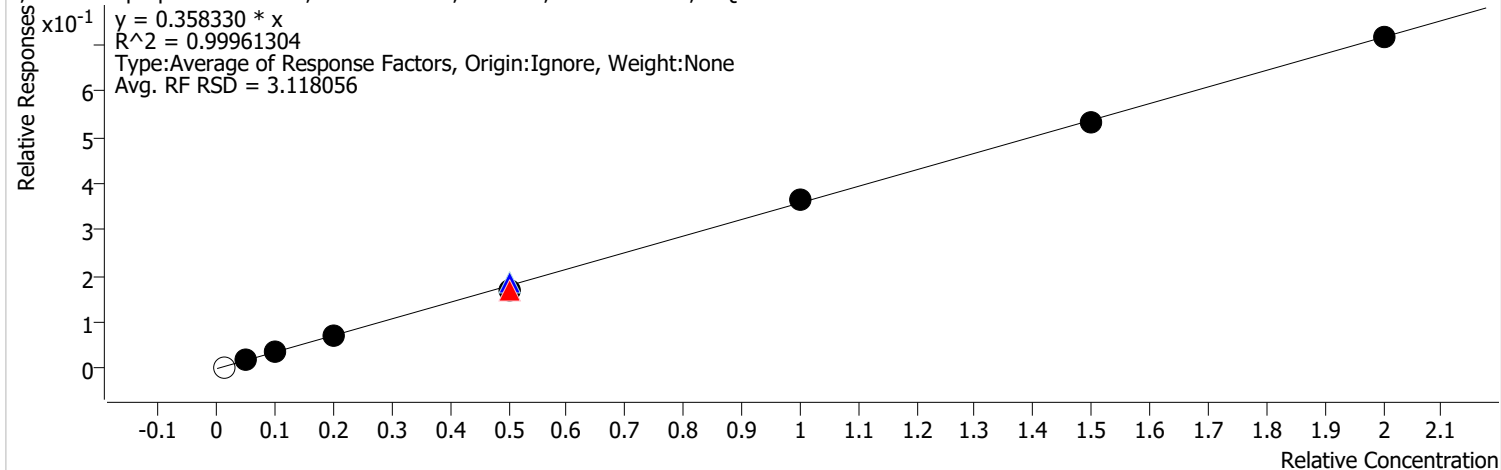


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 2930   | 2.5000    | 0.3801       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 13676  | 12.5000   | 0.3578       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 29793  | 25.0000   | 0.3765       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 56189  | 50.0000   | 0.3611       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 150902 | 125.0000  | 0.3767       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 139656 | 125.0000  | 0.3392       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 139656 | 125.0000  | 0.3392       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 303307 | 250.0000  | 0.3627       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 446282 | 375.0000  | 0.3534       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 601823 | 500.0000  | 0.3576       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:43 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**cis-1,2-Dichloroethene %RSE = 4.1**

cis-1,2-Dichloroethene - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs

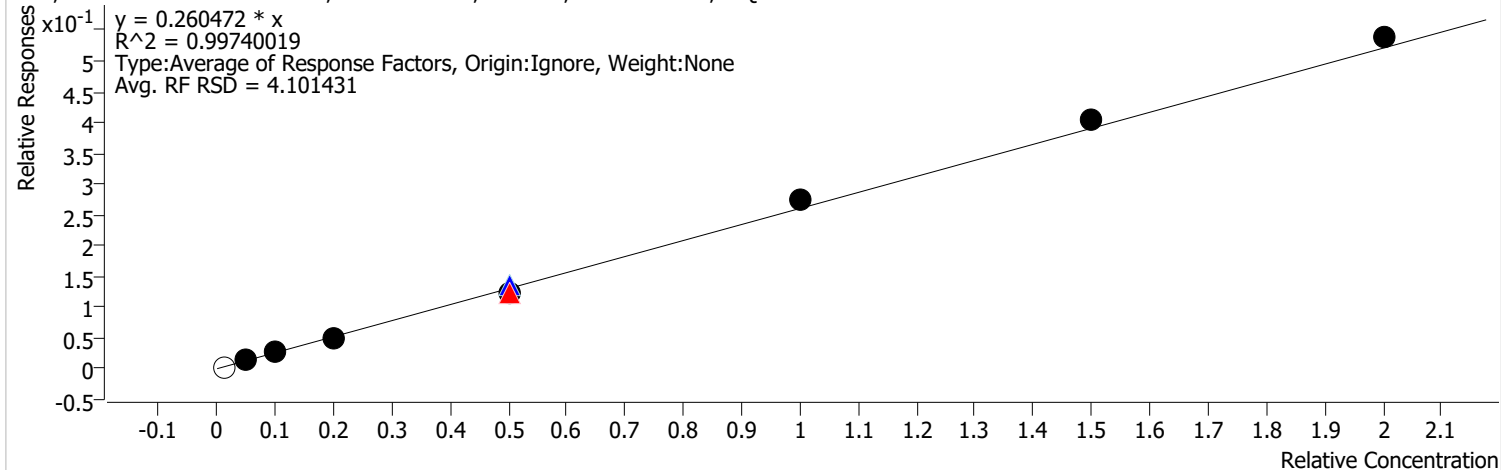


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 2376   | 2.5000    | 0.3082       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 10008  | 12.5000   | 0.2618       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 20252  | 25.0000   | 0.2559       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 39251  | 50.0000   | 0.2522       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 108623 | 125.0000  | 0.2711       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 100057 | 125.0000  | 0.2430       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 100057 | 125.0000  | 0.2430       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 228170 | 250.0000  | 0.2728       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 339211 | 375.0000  | 0.2686       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 452377 | 500.0000  | 0.2688       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:43 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**Methyl ethyl ketone %RSE = 6.4**

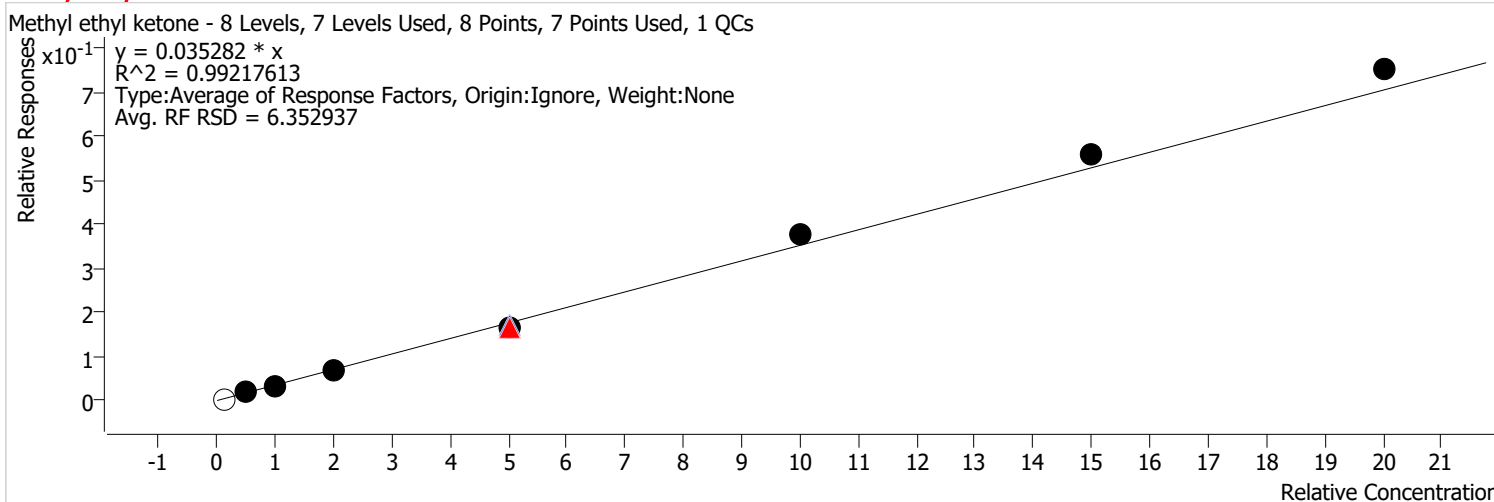


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 3035   | 25.0000   | 0.0394       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 13167  | 125.0000  | 0.0344       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 26248  | 250.0000  | 0.0332       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 52648  | 500.0000  | 0.0338       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 135511 | 1250.0000 | 0.0338       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 134730 | 1250.0000 | 0.0327       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 134730 | 1250.0000 | 0.0327       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 317271 | 2500.0000 | 0.0379       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 470653 | 3750.0000 | 0.0373       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 632539 | 5000.0000 | 0.0376       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:43 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**Bromochloromethane %RSE = 3.2**

Bromochloromethane - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs




| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 807    | 2.5000    | 0.1047       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 4275   | 12.5000   | 0.1118       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 8688   | 25.0000   | 0.1098       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 17338  | 50.0000   | 0.1114       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 42744  | 125.0000  | 0.1067       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 41966  | 125.0000  | 0.1019       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 41966  | 125.0000  | 0.1019       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 89178  | 250.0000  | 0.1066       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 135103 | 375.0000  | 0.1070       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 179618 | 500.0000  | 0.1067       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:43 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**Chloroform %RSE = 7.3**

Chloroform - 8 Levels, 8 Levels Used, 8 Points, 8 Points Used, 1 QCs

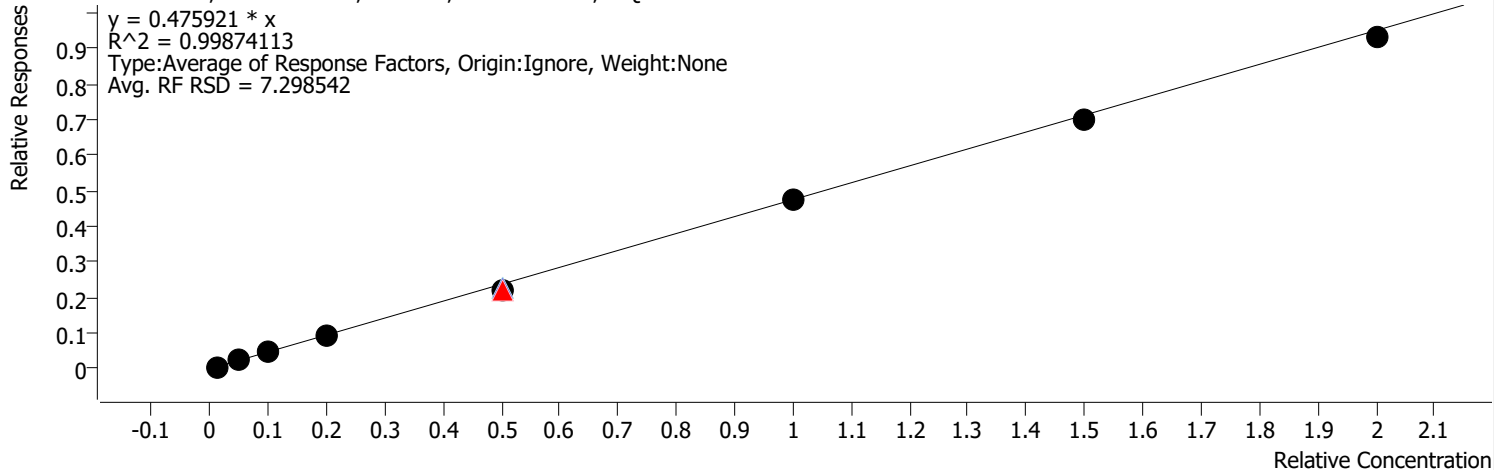


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     | x       | 4248   | 2.5000    | 0.5510       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 19015  | 12.5000   | 0.4975       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 36413  | 25.0000   | 0.4602       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 71403  | 50.0000   | 0.4588       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 183676 | 125.0000  | 0.4585       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 179640 | 125.0000  | 0.4363       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 179640 | 125.0000  | 0.4363       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 394946 | 250.0000  | 0.4723       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 588080 | 375.0000  | 0.4657       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 783422 | 500.0000  | 0.4656       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:43 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**1,1,1-Trichloroethane %RSE = 3.7**

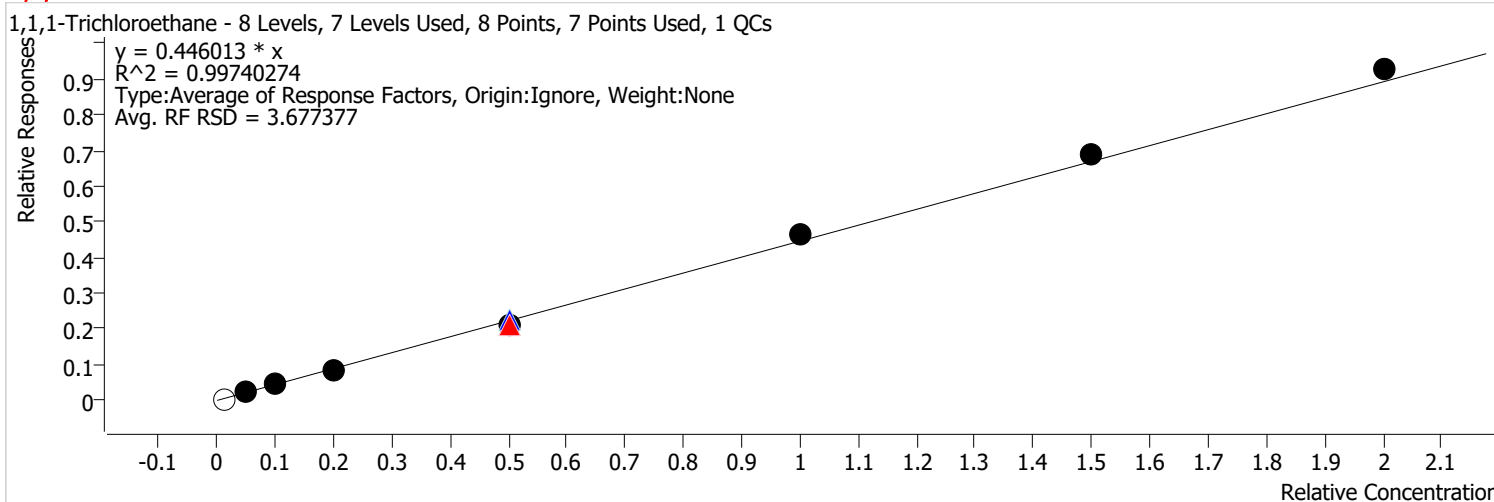


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 3510   | 2.5000    | 0.4553       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 16623  | 12.5000   | 0.4349       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 35547  | 25.0000   | 0.4492       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 67007  | 50.0000   | 0.4306       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 183324 | 125.0000  | 0.4576       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 174206 | 125.0000  | 0.4231       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 174206 | 125.0000  | 0.4231       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 386005 | 250.0000  | 0.4616       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 580748 | 375.0000  | 0.4599       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 778785 | 500.0000  | 0.4628       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:43 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**Dibromofluoromethane %RSE =**

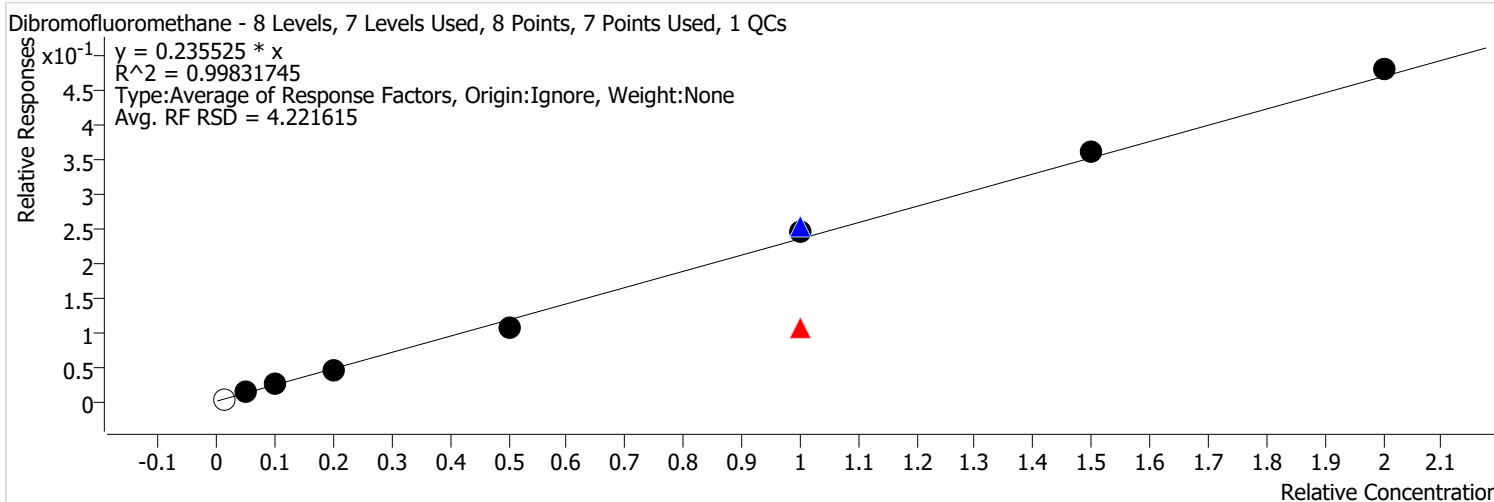


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 2508   | 2.5000    | 0.3253       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 9074   | 12.5000   | 0.2374       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 19100  | 25.0000   | 0.2414       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 35309  | 50.0000   | 0.2269       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 89307  | 125.0000  | 0.2169       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 204707 | 250.0000  | 0.2555       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 204073 | 250.0000  | 0.2440       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 89307  | 250.0000  | 0.1084       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 305158 | 375.0000  | 0.2416       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 404568 | 500.0000  | 0.2404       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:43 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**Carbon tetrachloride %RSE = 3.9**

Carbon tetrachloride - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs

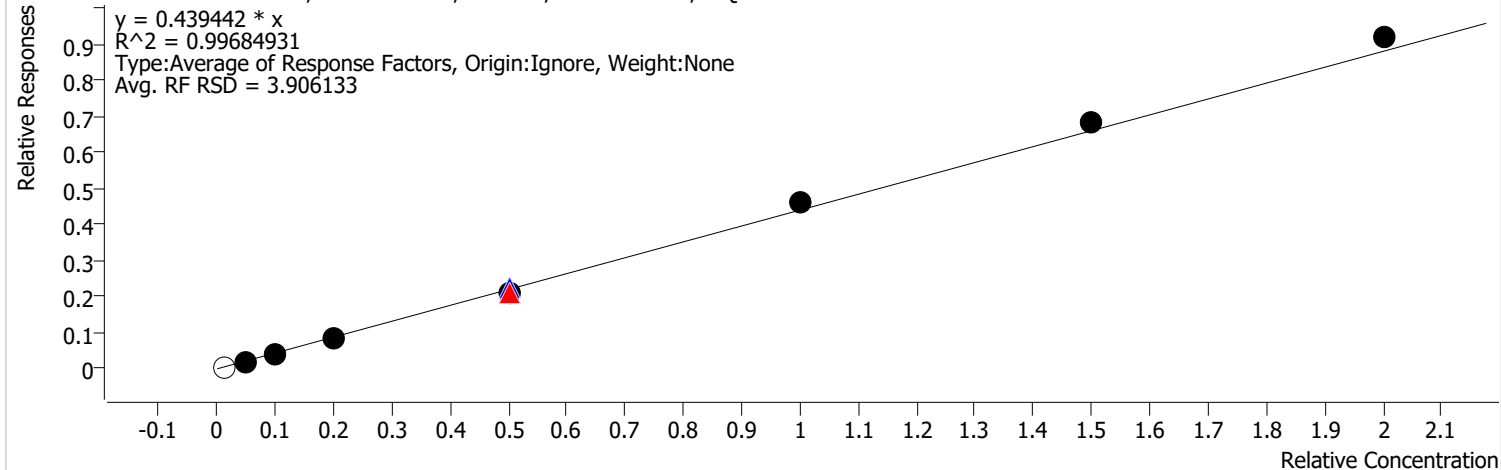


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 4342   | 2.5000    | 0.5632       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 16466  | 12.5000   | 0.4308       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 34462  | 25.0000   | 0.4355       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 65313  | 50.0000   | 0.4197       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 181384 | 125.0000  | 0.4528       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 172928 | 125.0000  | 0.4200       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 172928 | 125.0000  | 0.4200       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 383485 | 250.0000  | 0.4586       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 572545 | 375.0000  | 0.4534       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 770907 | 500.0000  | 0.4581       |           |



# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:44 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**1,1-Dichloropropene %RSE = 6.8**

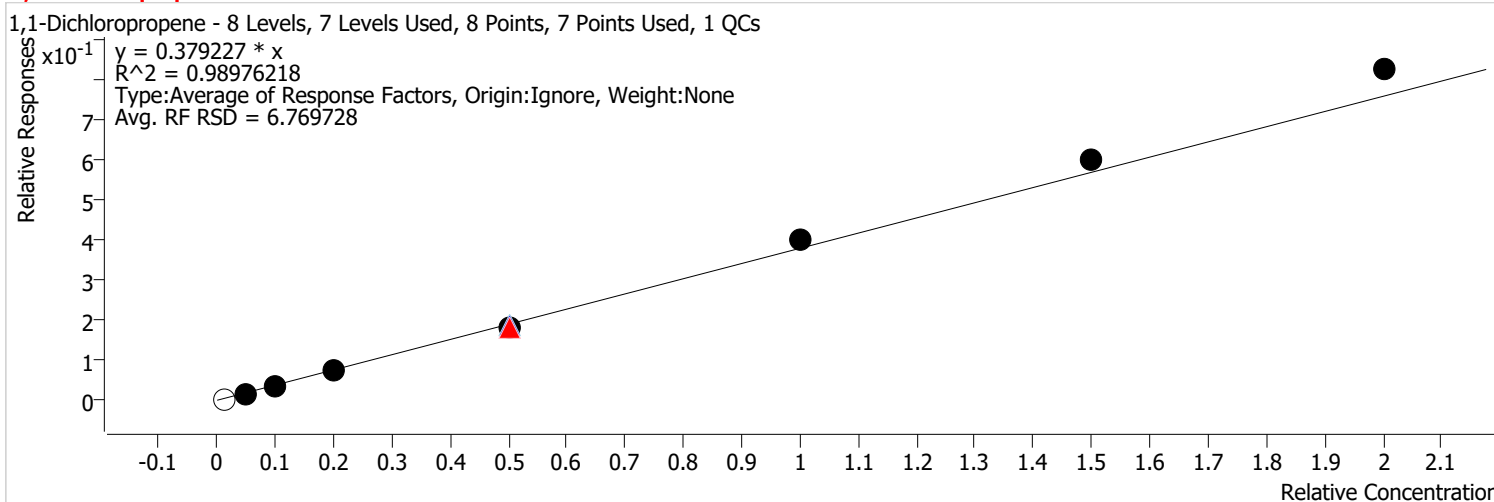


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 2830   | 2.5000    | 0.3671       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 13149  | 12.5000   | 0.3440       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 29241  | 25.0000   | 0.3695       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 56376  | 50.0000   | 0.3623       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 150930 | 125.0000  | 0.3768       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 149649 | 125.0000  | 0.3635       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 149649 | 125.0000  | 0.3635       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 335741 | 250.0000  | 0.4015       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 507157 | 375.0000  | 0.4016       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 693669 | 500.0000  | 0.4122       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:44 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**1,2-Dichloroethane-d4 %RSE =**

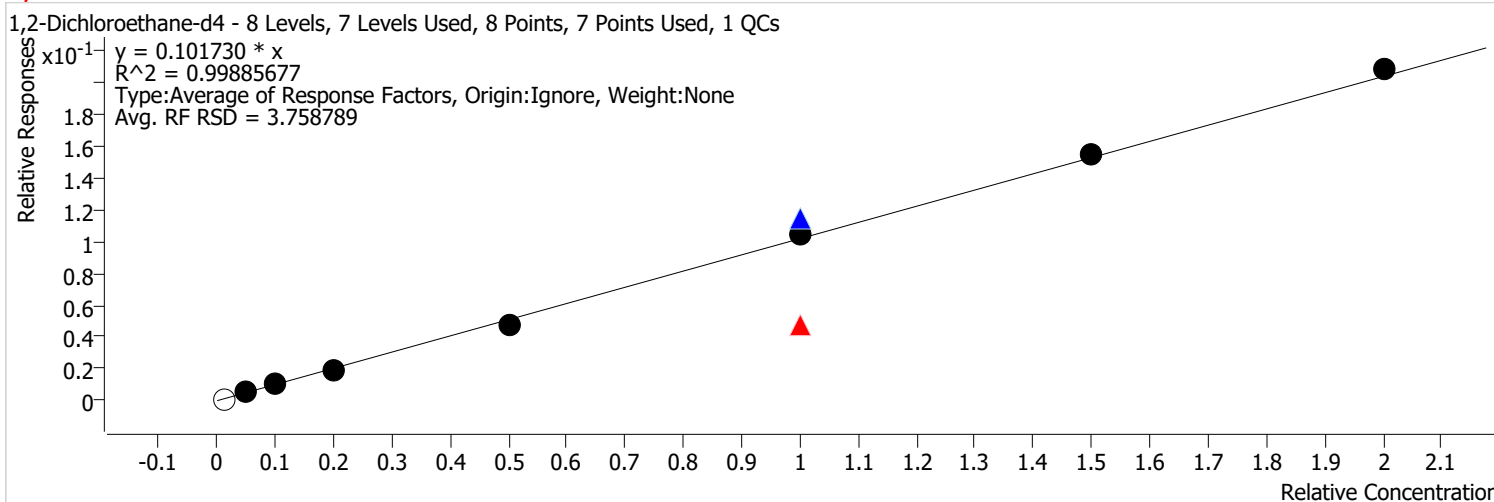


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 923    | 2.5000    | 0.1198       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 3938   | 12.5000   | 0.1030       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 8284   | 25.0000   | 0.1047       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 15238  | 50.0000   | 0.0979       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 39086  | 125.0000  | 0.0949       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 91382  | 250.0000  | 0.1141       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 87876  | 250.0000  | 0.1051       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 39086  | 250.0000  | 0.0475       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 129608 | 375.0000  | 0.1026       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 174713 | 500.0000  | 0.1038       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:44 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**Benzene %RSE = 5.4**

Benzene - 8 Levels, 8 Levels Used, 8 Points, 8 Points Used, 1 QCs

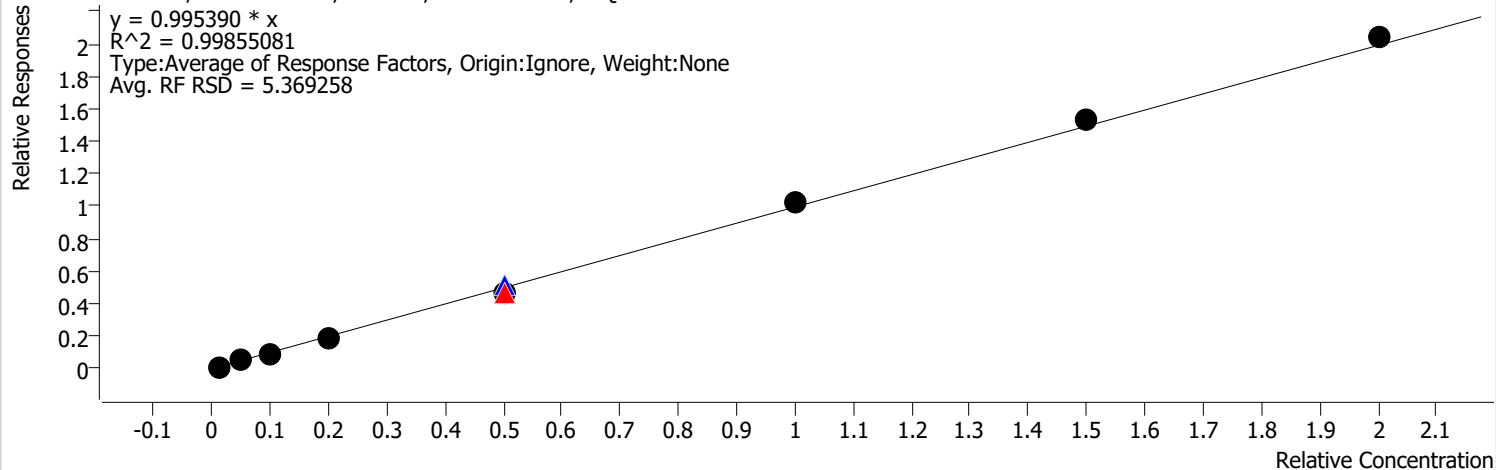


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.   | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|---------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     | x       | 8408    | 2.5000    | 1.0907       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 37071   | 12.5000   | 0.9699       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 74956   | 25.0000   | 0.9473       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 148727  | 50.0000   | 0.9557       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 418900  | 125.0000  | 1.0457       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 383469  | 125.0000  | 0.9313       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 383469  | 125.0000  | 0.9313       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 857534  | 250.0000  | 1.0254       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 1293370 | 375.0000  | 1.0242       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 1714050 | 500.0000  | 1.0186       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:44 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**1,2-Dichloroethane %RSE = 7.0**

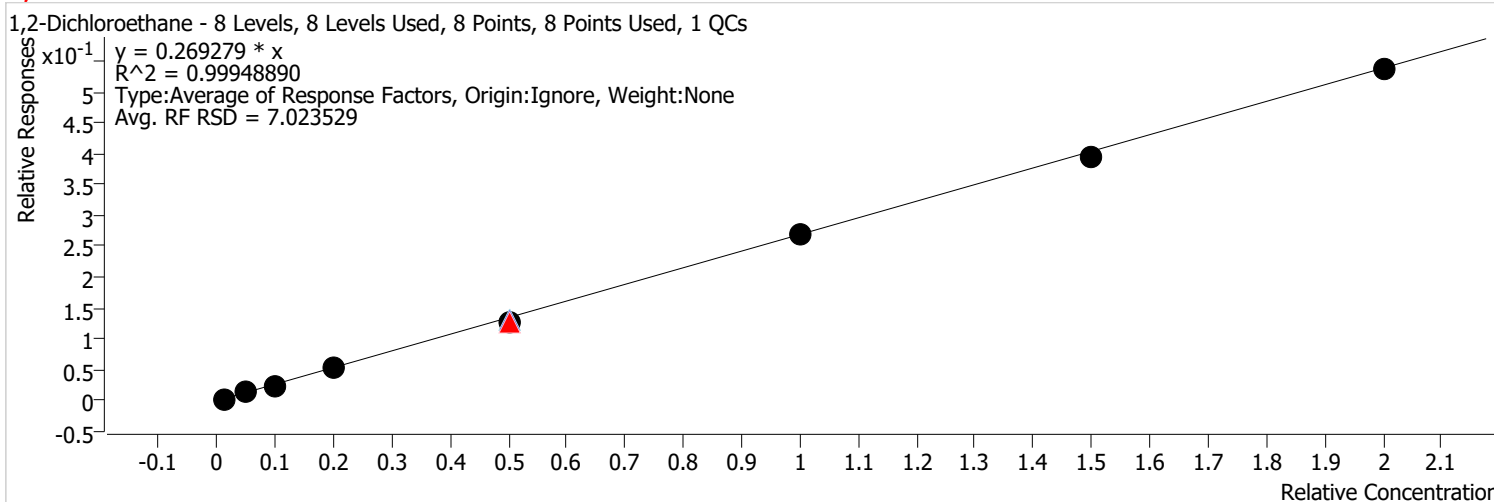


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     | x       | 2415   | 2.5000    | 0.3133       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 10202  | 12.5000   | 0.2669       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 19996  | 25.0000   | 0.2527       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 41058  | 50.0000   | 0.2638       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 104249 | 125.0000  | 0.2602       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 104855 | 125.0000  | 0.2547       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 104855 | 125.0000  | 0.2547       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 226964 | 250.0000  | 0.2714       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 332775 | 375.0000  | 0.2635       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 450739 | 500.0000  | 0.2679       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:44 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**Trichloroethene %RSE = 5.6**

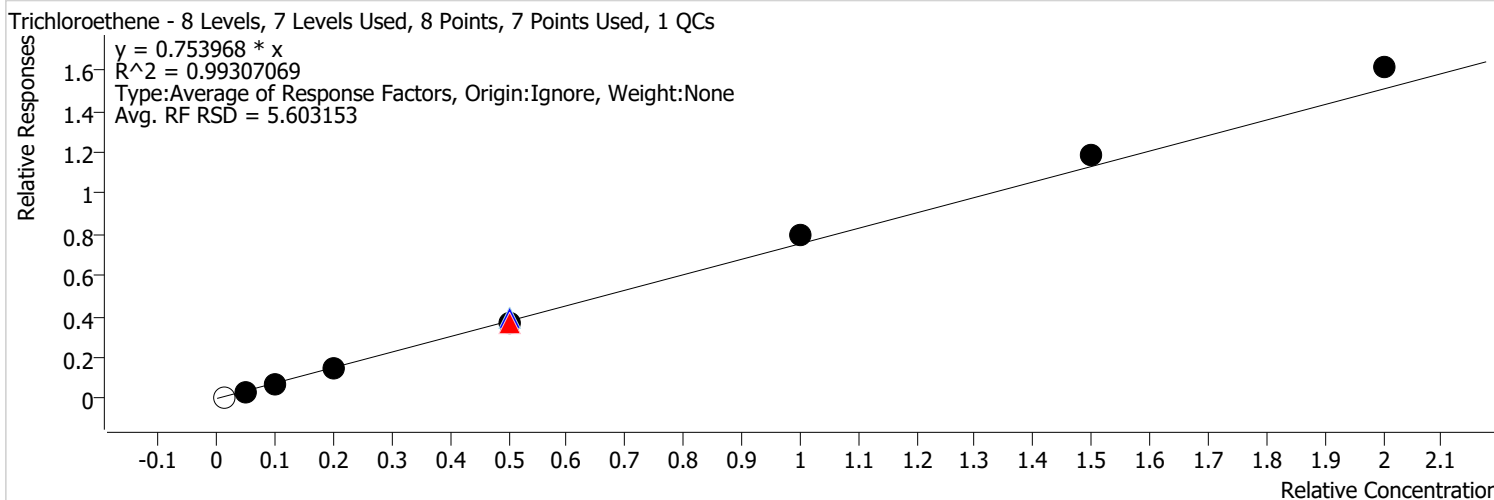


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 2372   | 2.5000    | 0.8011       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 10442  | 12.5000   | 0.7042       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 21946  | 25.0000   | 0.7283       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 42682  | 50.0000   | 0.7105       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 121734 | 125.0000  | 0.7908       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 114123 | 125.0000  | 0.7447       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 114123 | 125.0000  | 0.7447       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 250285 | 250.0000  | 0.7910       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 374370 | 375.0000  | 0.7932       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 505400 | 500.0000  | 0.8058       |           |

# Calibration Report

|                     |                                                                     |                      |                |
|---------------------|---------------------------------------------------------------------|----------------------|----------------|
| Batch Path          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name         | BL2000\mchavez |
| Analysis Time       | 2/28/2022 1:57 PM                                                   | Reporter Name        | BL2000\mchavez |
| Report Time         | 2/28/2022 2:00:44 PM                                                | Batch State          | Processed      |
| Last Calib Update   | 1/9/2022 8:59 PM                                                    | Quant Report Version | 10.0           |
| Quant Batch Version | 10.0                                                                |                      |                |

**1,2-Dichloropropane %RSE = 3.7**

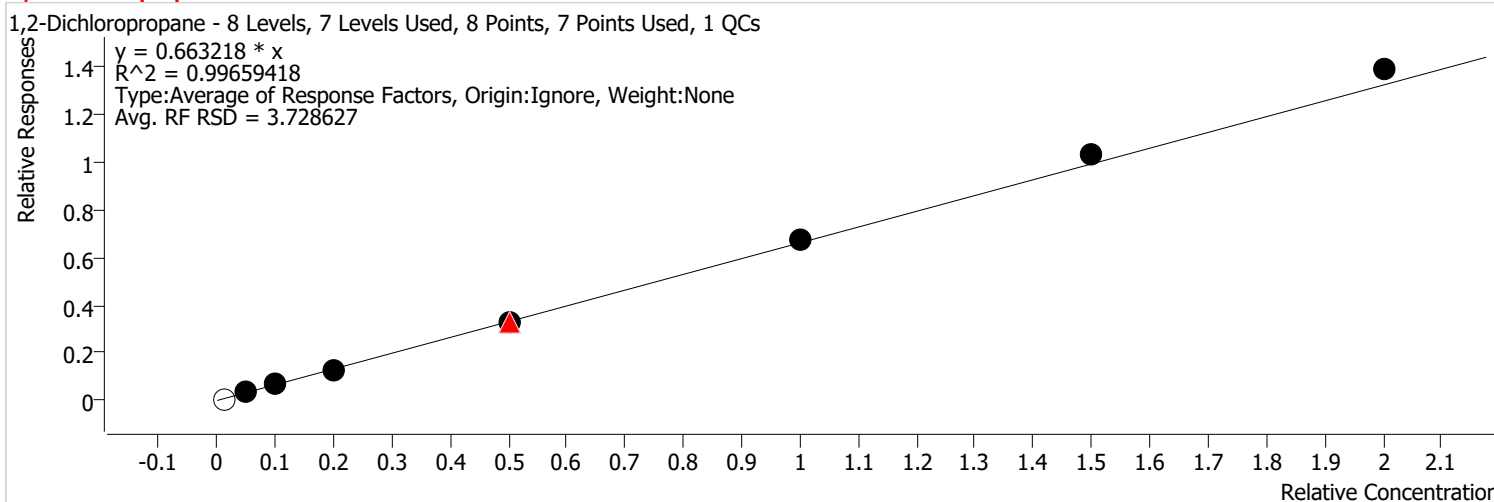


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 2148   | 2.5000    | 0.7255       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 9488   | 12.5000   | 0.6399       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 20077  | 25.0000   | 0.6663       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 37870  | 50.0000   | 0.6304       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 102633 | 125.0000  | 0.6667       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 99187  | 125.0000  | 0.6472       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 99187  | 125.0000  | 0.6472       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 213800 | 250.0000  | 0.6757       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 324602 | 375.0000  | 0.6877       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 436057 | 500.0000  | 0.6953       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:44 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**Dibromomethane %RSE = 6.3**

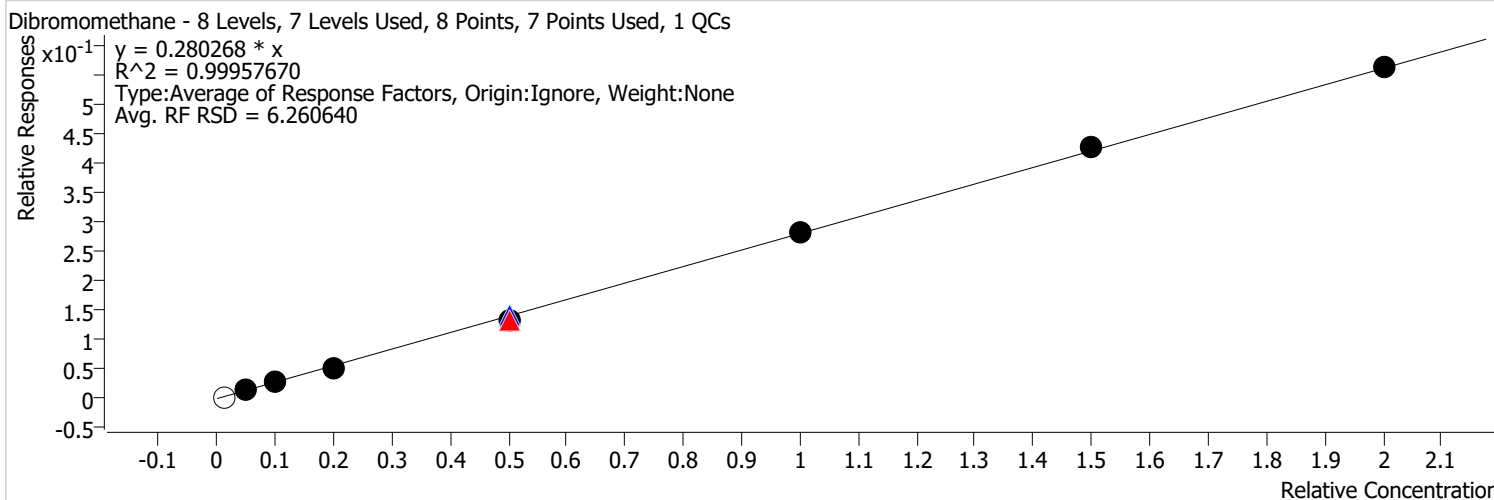


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 902    | 2.5000    | 0.3045       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 4675   | 12.5000   | 0.3153       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 8055   | 25.0000   | 0.2673       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 15989  | 50.0000   | 0.2662       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 43248  | 125.0000  | 0.2810       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 40628  | 125.0000  | 0.2651       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 40628  | 125.0000  | 0.2651       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 89483  | 250.0000  | 0.2828       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 134282 | 375.0000  | 0.2845       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 176038 | 500.0000  | 0.2807       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:44 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**Bromodichloromethane %RSE = 3.5**

Bromodichloromethane - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs

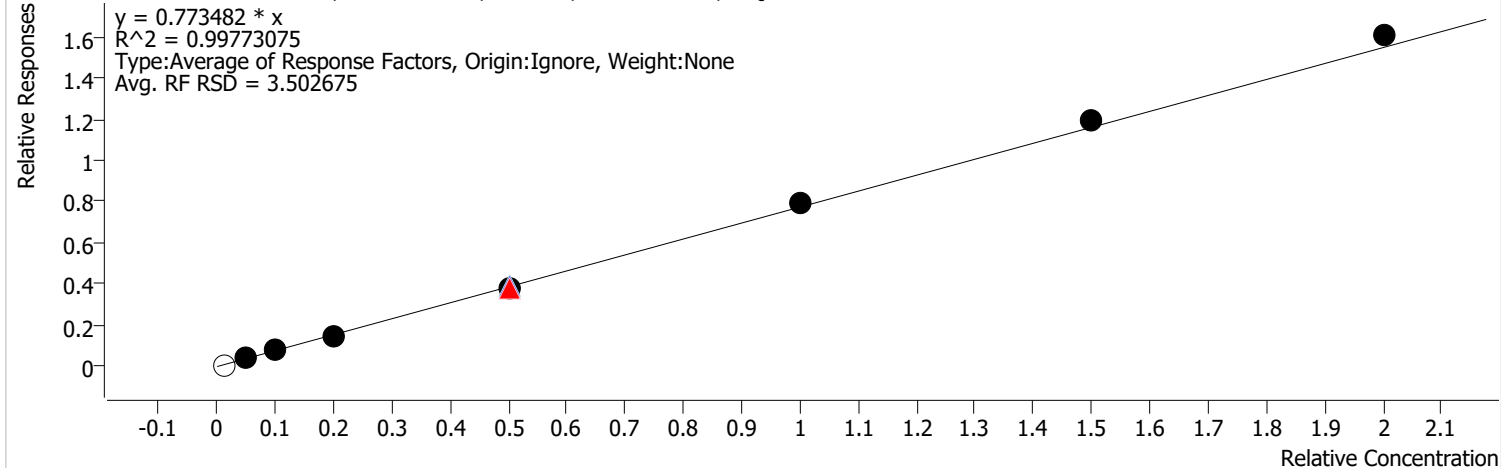

| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 2536   | 2.5000    | 0.8565       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 11562  | 12.5000   | 0.7798       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 22743  | 25.0000   | 0.7547       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 43900  | 50.0000   | 0.7308       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 122757 | 125.0000  | 0.7975       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 115664 | 125.0000  | 0.7548       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 115664 | 125.0000  | 0.7548       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 251805 | 250.0000  | 0.7958       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 375983 | 375.0000  | 0.7966       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 502929 | 500.0000  | 0.8019       |           |




# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:44 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**cis-1,3-Dichloropropene %RSE = 6.7**

cis-1,3-Dichloropropene - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs

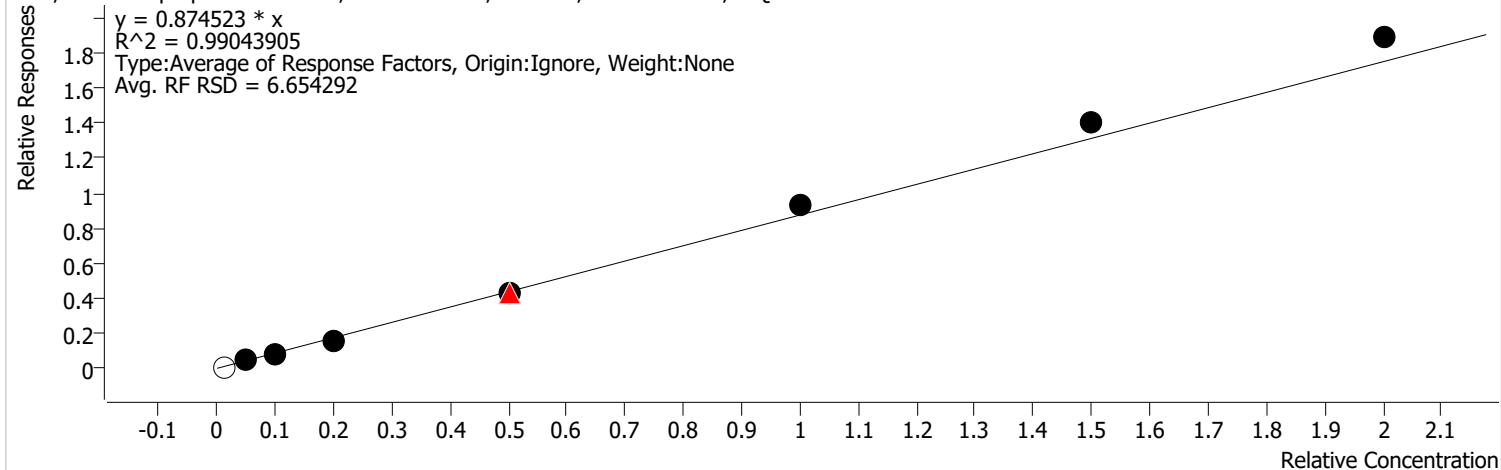


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 2583   | 2.5000    | 0.8724       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 12525  | 12.5000   | 0.8447       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 24511  | 25.0000   | 0.8134       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 48886  | 50.0000   | 0.8138       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 130910 | 125.0000  | 0.8504       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 129419 | 125.0000  | 0.8445       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 129419 | 125.0000  | 0.8445       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 293617 | 250.0000  | 0.9280       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 441168 | 375.0000  | 0.9347       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 591147 | 500.0000  | 0.9426       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:44 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**Toluene-d8 %RSE =**

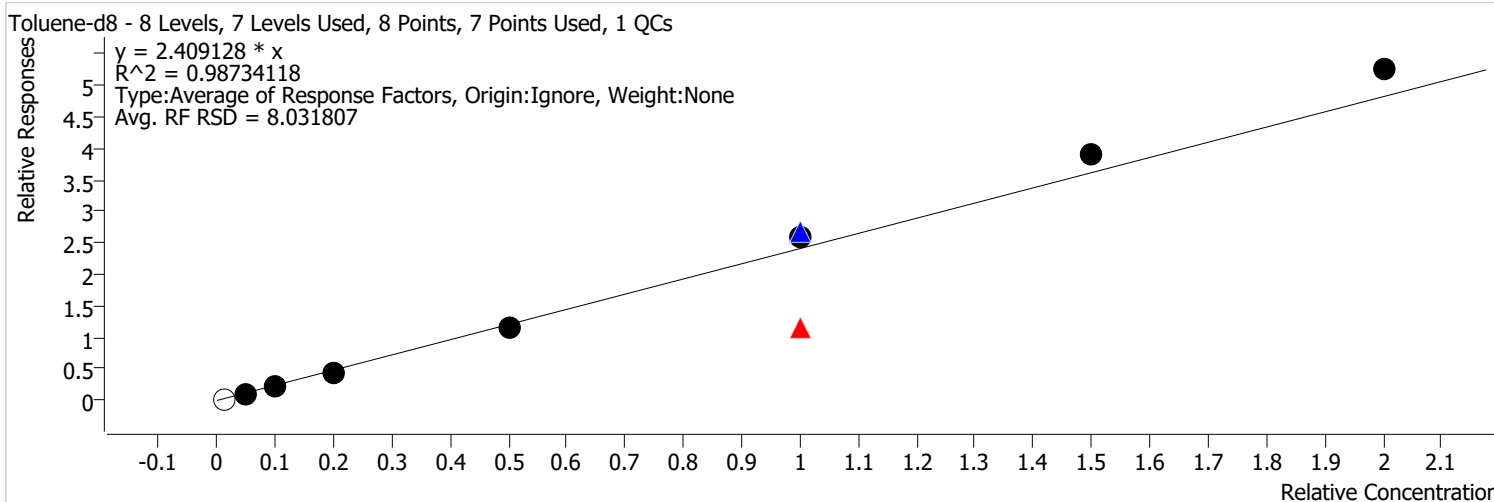


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.   | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|---------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 7777    | 2.5000    | 2.6266       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 32318   | 12.5000   | 2.1796       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 67673   | 25.0000   | 2.2458       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 136453  | 50.0000   | 2.2715       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 358186  | 125.0000  | 2.3373       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 821531  | 250.0000  | 2.6685       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 823306  | 250.0000  | 2.6021       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 358186  | 250.0000  | 1.1687       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 1229775 | 375.0000  | 2.6054       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 1644540 | 500.0000  | 2.6222       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:44 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**Toluene %RSE = 6.5**

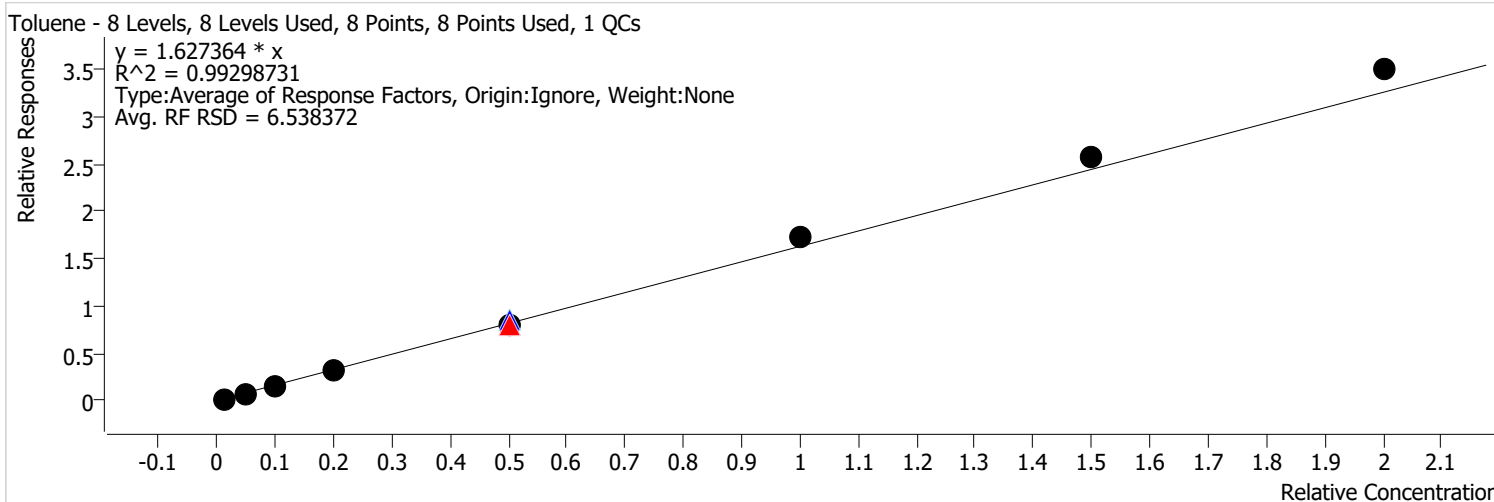


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.   | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|---------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     | x       | 5039    | 2.5000    | 1.7019       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 21794   | 12.5000   | 1.4698       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 46355   | 25.0000   | 1.5383       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 91915   | 50.0000   | 1.5301       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 264584  | 125.0000  | 1.7188       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 244712  | 125.0000  | 1.5969       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 244712  | 125.0000  | 1.5969       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 541945  | 250.0000  | 1.7129       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 813204  | 375.0000  | 1.7229       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 1095161 | 500.0000  | 1.7462       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:44 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**trans-1,3-Dichloropropene %RSE = 6.2**

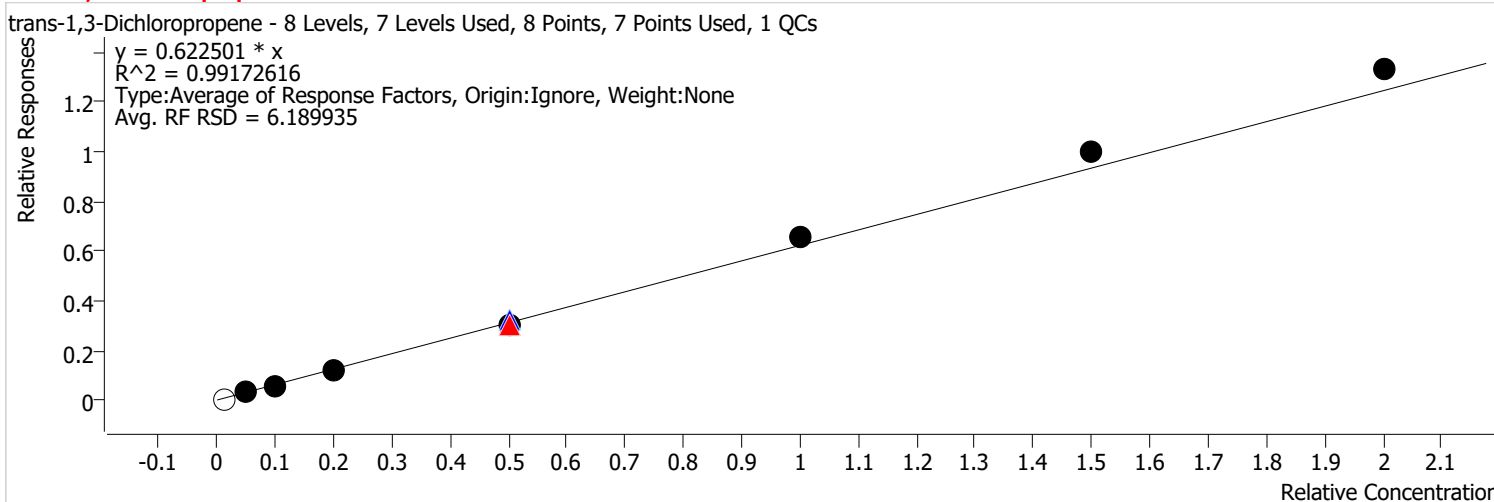


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 1470   | 2.5000    | 0.4966       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 8683   | 12.5000   | 0.5856       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 17850  | 25.0000   | 0.5924       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 35179  | 50.0000   | 0.5856       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 98907  | 125.0000  | 0.6425       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 92719  | 125.0000  | 0.6050       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 92719  | 125.0000  | 0.6050       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 207833 | 250.0000  | 0.6569       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 315063 | 375.0000  | 0.6675       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 416771 | 500.0000  | 0.6645       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:44 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**1,1,2-Trichloroethane %RSE = 4.0**

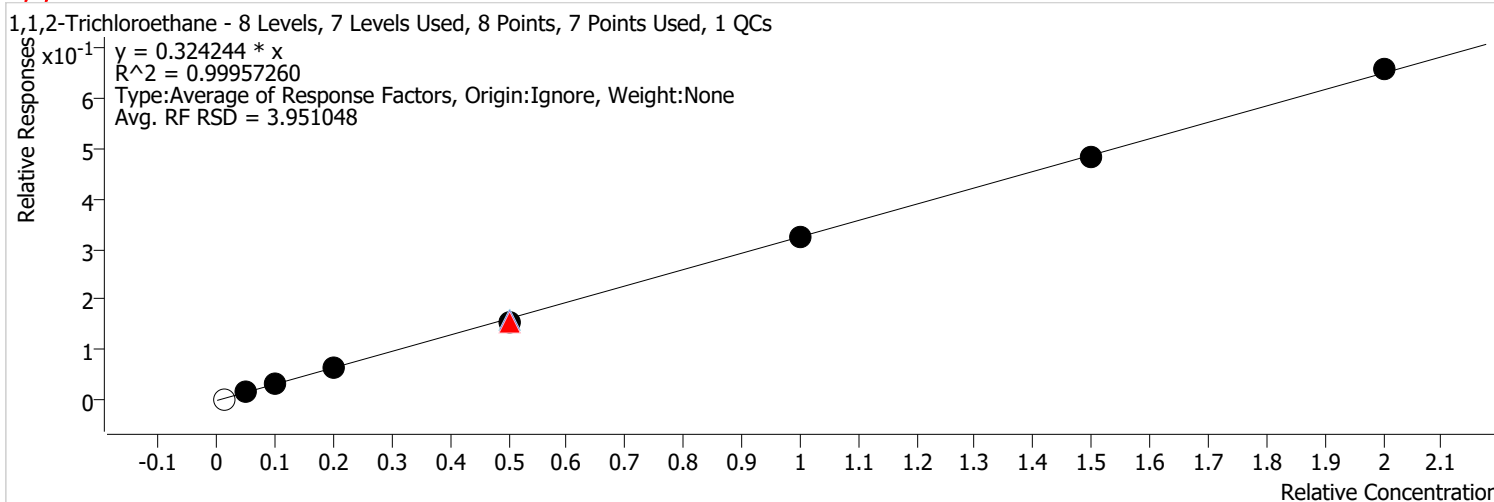


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 960    | 2.5000    | 0.3244       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 5090   | 12.5000   | 0.3433       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 10099  | 25.0000   | 0.3351       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 18884  | 50.0000   | 0.3144       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 49128  | 125.0000  | 0.3191       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 46673  | 125.0000  | 0.3046       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 46673  | 125.0000  | 0.3046       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 101888 | 250.0000  | 0.3220       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 152331 | 375.0000  | 0.3227       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 205463 | 500.0000  | 0.3276       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:44 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**Tetrachloroethene %RSE = 5.2**

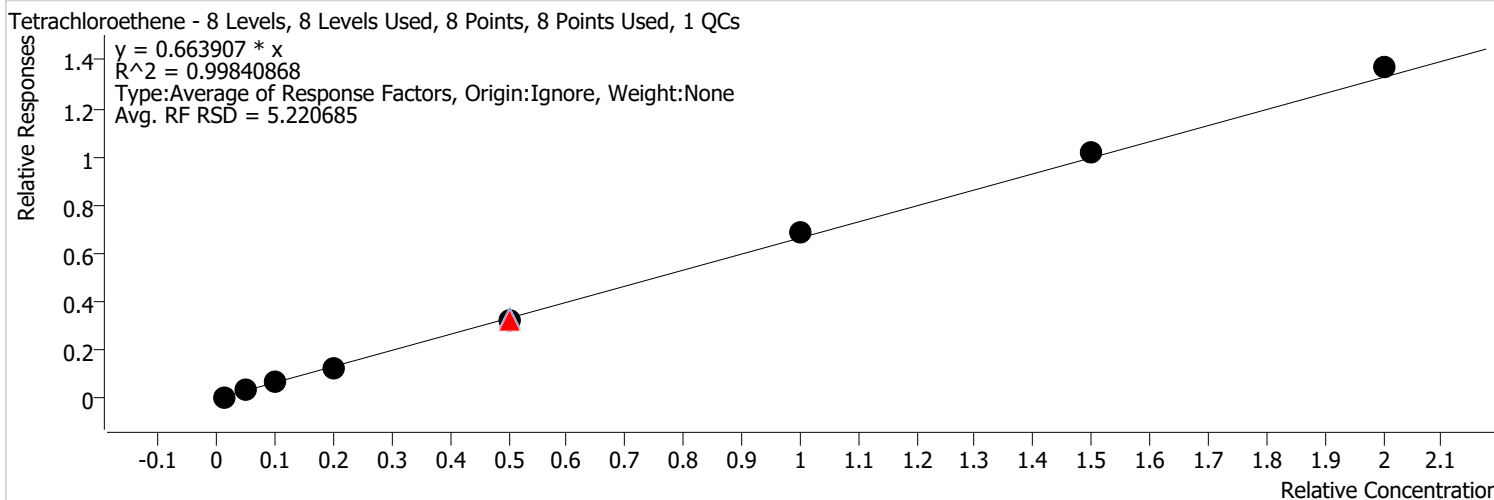


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     | x       | 2105   | 2.5000    | 0.7110       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 9238   | 12.5000   | 0.6230       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 20322  | 25.0000   | 0.6744       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 36925  | 50.0000   | 0.6147       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 103027 | 125.0000  | 0.6693       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 97590  | 125.0000  | 0.6368       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 97590  | 125.0000  | 0.6368       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 218245 | 250.0000  | 0.6898       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 319950 | 375.0000  | 0.6779       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 428812 | 500.0000  | 0.6837       |           |

# Calibration Report

|                     |                                                                     |                      |                |
|---------------------|---------------------------------------------------------------------|----------------------|----------------|
| Batch Path          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name         | BL2000\mchavez |
| Analysis Time       | 2/28/2022 1:57 PM                                                   | Reporter Name        | BL2000\mchavez |
| Report Time         | 2/28/2022 2:00:44 PM                                                | Batch State          | Processed      |
| Last Calib Update   | 1/9/2022 8:59 PM                                                    | Quant Report Version | 10.0           |
| Quant Batch Version | 10.0                                                                |                      |                |

**1,3-Dichloropropane %RSE = 3.9**

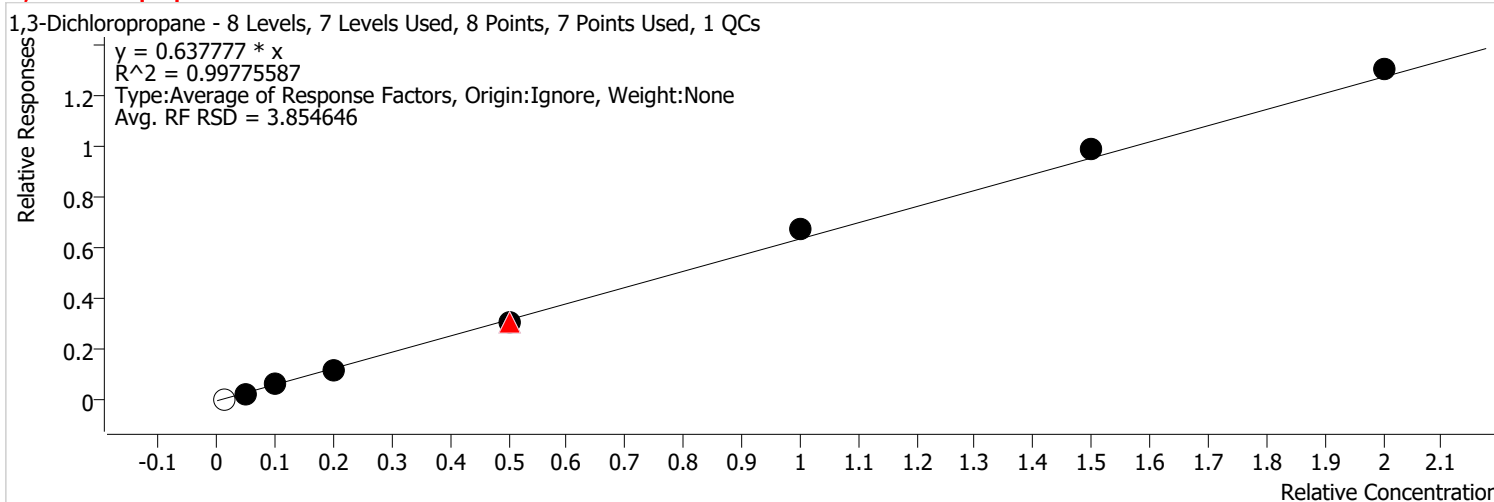


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 2257   | 2.5000    | 0.7623       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 8967   | 12.5000   | 0.6047       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 18745  | 25.0000   | 0.6221       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 37457  | 50.0000   | 0.6235       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 95697  | 125.0000  | 0.6217       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 96183  | 125.0000  | 0.6276       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 96183  | 125.0000  | 0.6276       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 212669 | 250.0000  | 0.6722       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 312547 | 375.0000  | 0.6622       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 408993 | 500.0000  | 0.6521       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:44 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**Chlorodibromomethane %RSE = 4.5**

Chlorodibromomethane - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs

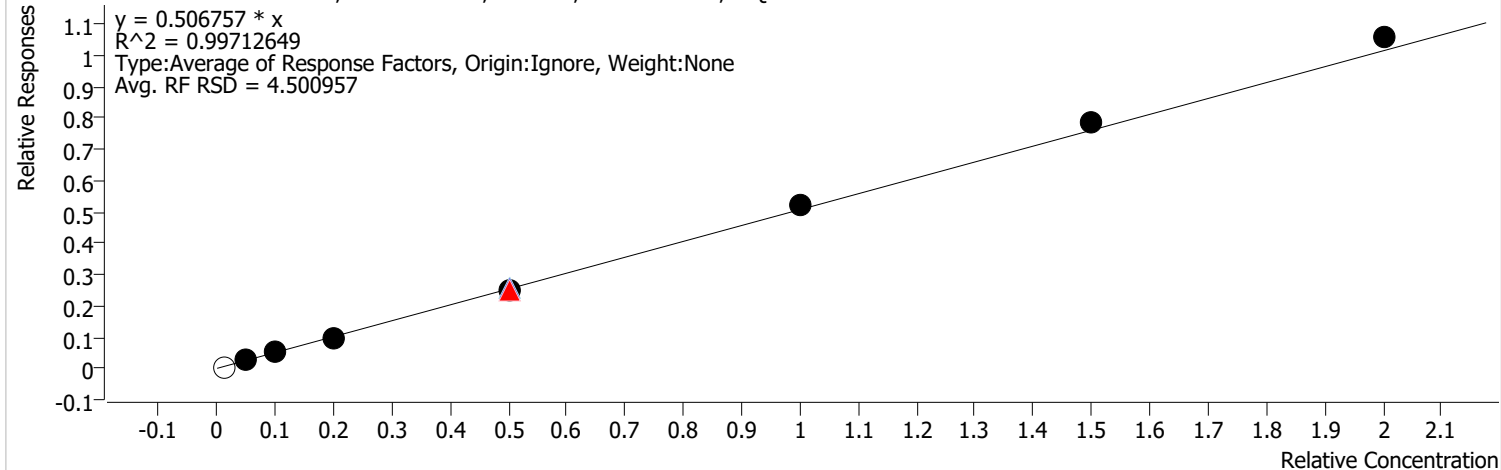


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 1468   | 2.5000    | 0.4958       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 7718   | 12.5000   | 0.5205       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 14873  | 25.0000   | 0.4936       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 28153  | 50.0000   | 0.4687       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 78076  | 125.0000  | 0.5072       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 75015  | 125.0000  | 0.4895       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 75015  | 125.0000  | 0.4895       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 165695 | 250.0000  | 0.5237       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 247279 | 375.0000  | 0.5239       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 330813 | 500.0000  | 0.5275       |           |



# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:44 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**1,2-Dibromoethane %RSE = 2.9**

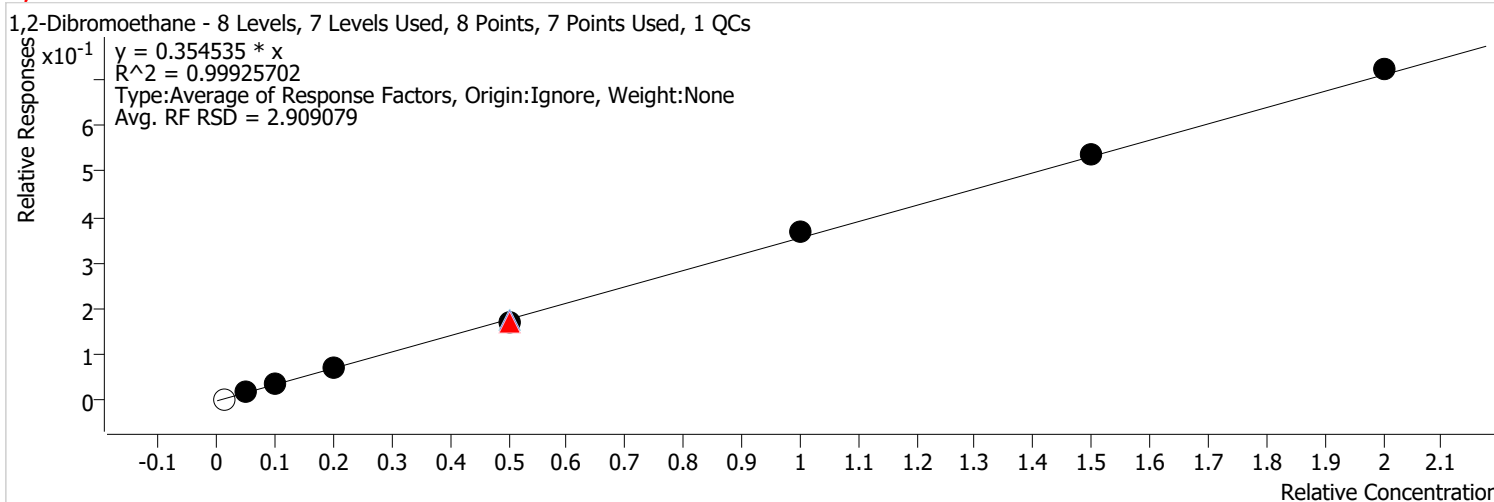


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 1299   | 2.5000    | 0.4388       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 5410   | 12.5000   | 0.3649       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 10410  | 25.0000   | 0.3455       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 21037  | 50.0000   | 0.3502       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 54259  | 125.0000  | 0.3525       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 51827  | 125.0000  | 0.3382       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 51827  | 125.0000  | 0.3382       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 115714 | 250.0000  | 0.3657       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 168577 | 375.0000  | 0.3572       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 225877 | 500.0000  | 0.3602       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:44 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**Chlorobenzene %RSE = 3.5**

Chlorobenzene - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs

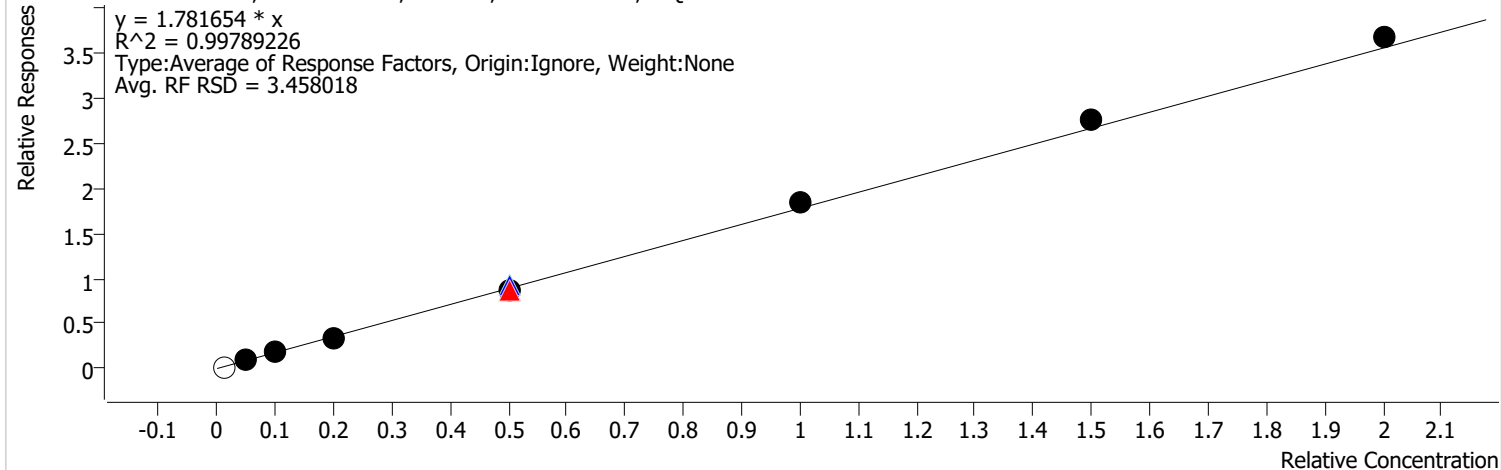


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.   | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|---------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 5771    | 2.5000    | 1.9491       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 26461   | 12.5000   | 1.7846       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 53047   | 25.0000   | 1.7604       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 101452  | 50.0000   | 1.6889       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 288815  | 125.0000  | 1.8762       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 263617  | 125.0000  | 1.7202       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 263617  | 125.0000  | 1.7202       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 582326  | 250.0000  | 1.8405       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 867732  | 375.0000  | 1.8384       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 1153147 | 500.0000  | 1.8387       |           |

# Calibration Report

|                     |                                                                     |                      |                |
|---------------------|---------------------------------------------------------------------|----------------------|----------------|
| Batch Path          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name         | BL2000\mchavez |
| Analysis Time       | 2/28/2022 1:57 PM                                                   | Reporter Name        | BL2000\mchavez |
| Report Time         | 2/28/2022 2:00:44 PM                                                | Batch State          | Processed      |
| Last Calib Update   | 1/9/2022 8:59 PM                                                    | Quant Report Version | 10.0           |
| Quant Batch Version | 10.0                                                                |                      |                |

**1,1,1,2-Tetrachloroethane %RSE = 4.2**

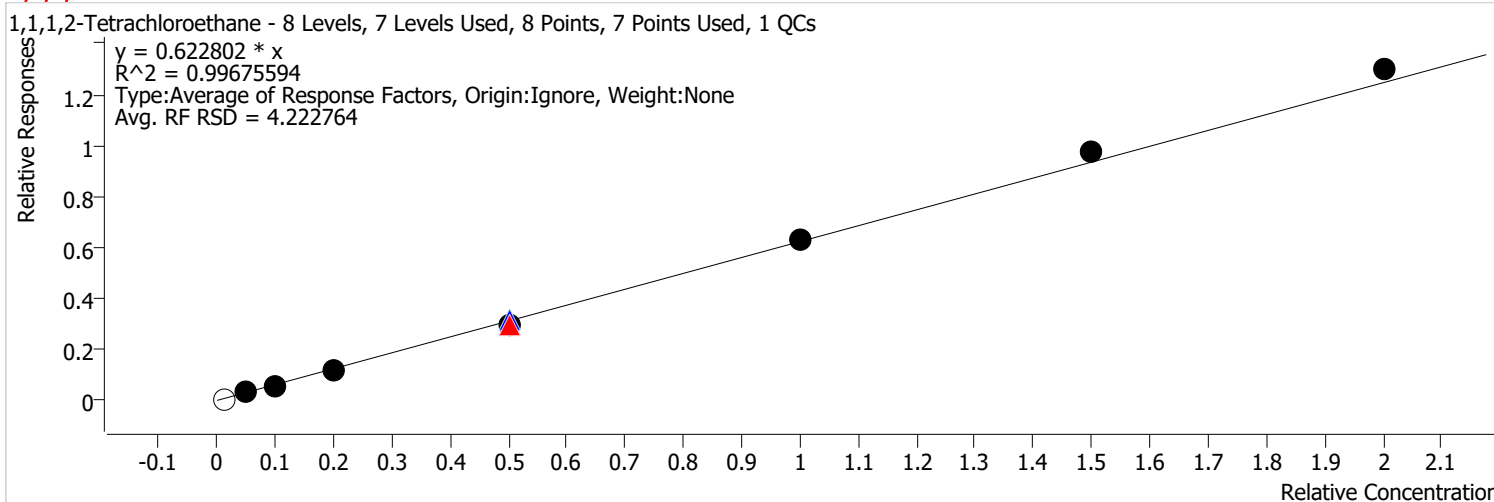


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 1893   | 2.5000    | 0.6392       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 9473   | 12.5000   | 0.6389       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 18130  | 25.0000   | 0.6016       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 35544  | 50.0000   | 0.5917       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 97148  | 125.0000  | 0.6311       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 90898  | 125.0000  | 0.5932       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 90898  | 125.0000  | 0.5932       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 200859 | 250.0000  | 0.6348       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 307436 | 375.0000  | 0.6513       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 406450 | 500.0000  | 0.6481       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:45 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**Ethylbenzene %RSE = 7.5**

Ethylbenzene - 8 Levels, 8 Levels Used, 8 Points, 8 Points Used, 1 QCs




| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.   | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|---------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     | x       | 9283    | 2.5000    | 3.1353       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 40470   | 12.5000   | 2.7294       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 88428   | 25.0000   | 2.9345       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 173769  | 50.0000   | 2.8927       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 501953  | 125.0000  | 3.2608       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 464148  | 125.0000  | 3.0288       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 464148  | 125.0000  | 3.0288       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 1043443 | 250.0000  | 3.2979       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 1574219 | 375.0000  | 3.3352       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 2111152 | 500.0000  | 3.3662       |           |

# Calibration Report

|                     |                                                                     |                      |                |
|---------------------|---------------------------------------------------------------------|----------------------|----------------|
| Batch Path          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name         | BL2000\mchavez |
| Analysis Time       | 2/28/2022 1:57 PM                                                   | Reporter Name        | BL2000\mchavez |
| Report Time         | 2/28/2022 2:00:45 PM                                                | Batch State          | Processed      |
| Last Calib Update   | 1/9/2022 8:59 PM                                                    | Quant Report Version | 10.0           |
| Quant Batch Version | 10.0                                                                |                      |                |

**m+p-Xylenes %RSE = 8.3**

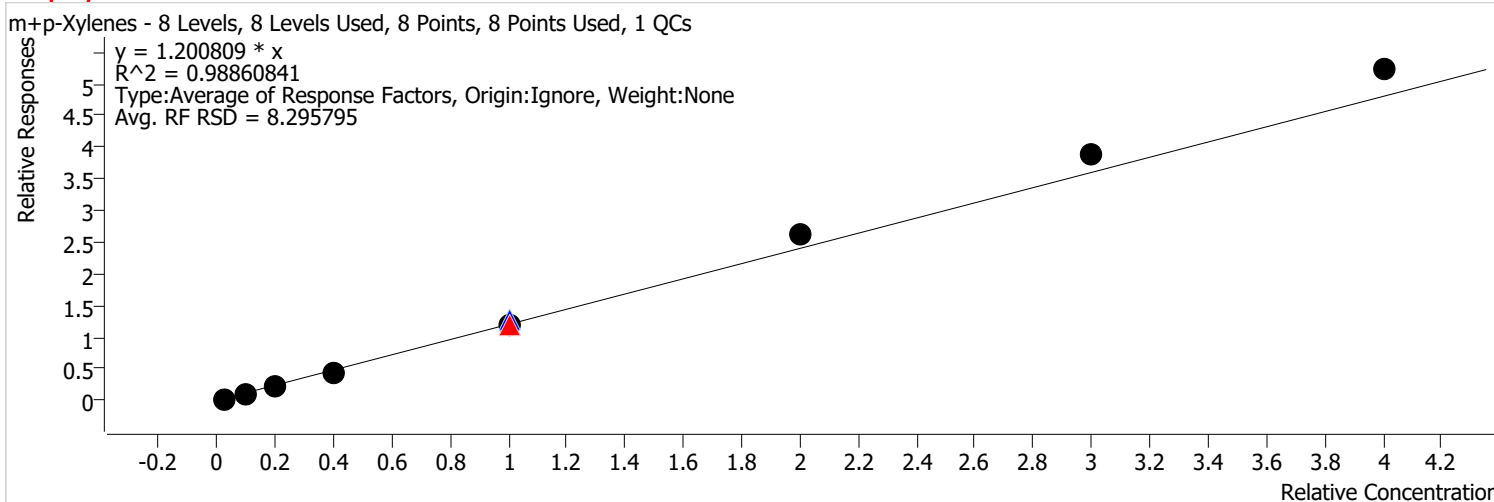


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.   | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|---------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     | x       | 7212    | 5.0000    | 1.2179       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 31538   | 25.0000   | 1.0635       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 66267   | 50.0000   | 1.0995       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 133498  | 100.0000  | 1.1112       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 388558  | 250.0000  | 1.2621       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 368418  | 250.0000  | 1.2021       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 368418  | 250.0000  | 1.2021       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 825866  | 500.0000  | 1.3051       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 1228570 | 750.0000  | 1.3014       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 1637879 | 1000.0000 | 1.3058       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:45 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**o-Xylene %RSE = 9.2**

o-Xylene - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs

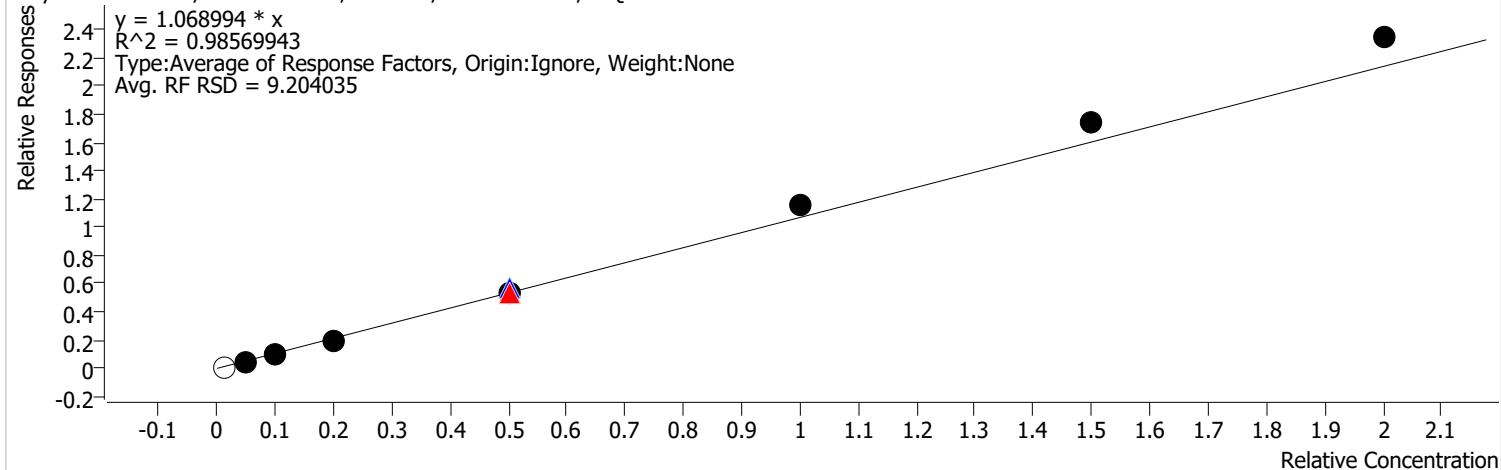


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 3330   | 2.5000    | 1.1247       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 13519  | 12.5000   | 0.9117       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 30463  | 25.0000   | 1.0109       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 61016  | 50.0000   | 1.0157       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 174061 | 125.0000  | 1.1308       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 161509 | 125.0000  | 1.0539       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 161509 | 125.0000  | 1.0539       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 365914 | 250.0000  | 1.1565       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 549244 | 375.0000  | 1.1636       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 734101 | 500.0000  | 1.1705       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:45 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**Styrene %RSE = 9.9**

Styrene - 8 Levels, 8 Levels Used, 8 Points, 8 Points Used, 1 QCs

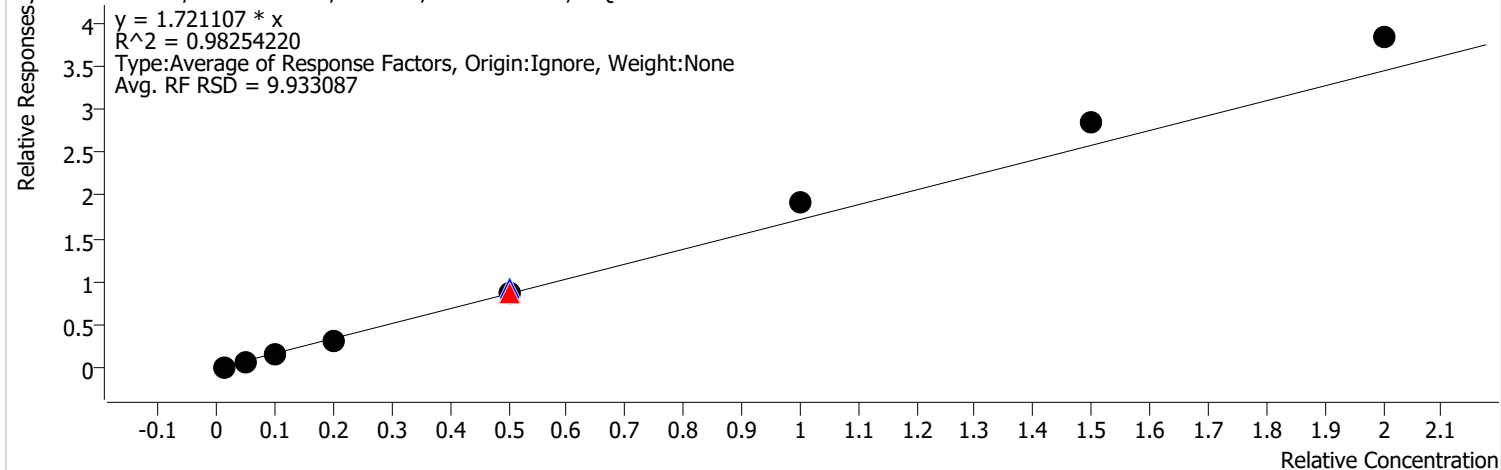


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.   | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|---------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     | x       | 4408    | 2.5000    | 1.4888       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 23472   | 12.5000   | 1.5830       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 48569   | 25.0000   | 1.6118       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 96576   | 50.0000   | 1.6077       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 291425  | 125.0000  | 1.8932       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 268375  | 125.0000  | 1.7513       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 268375  | 125.0000  | 1.7513       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 605646  | 250.0000  | 1.9142       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 896331  | 375.0000  | 1.8990       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 1199879 | 500.0000  | 1.9132       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:45 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**Bromoform %RSE = 4.7**

Bromoform - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs

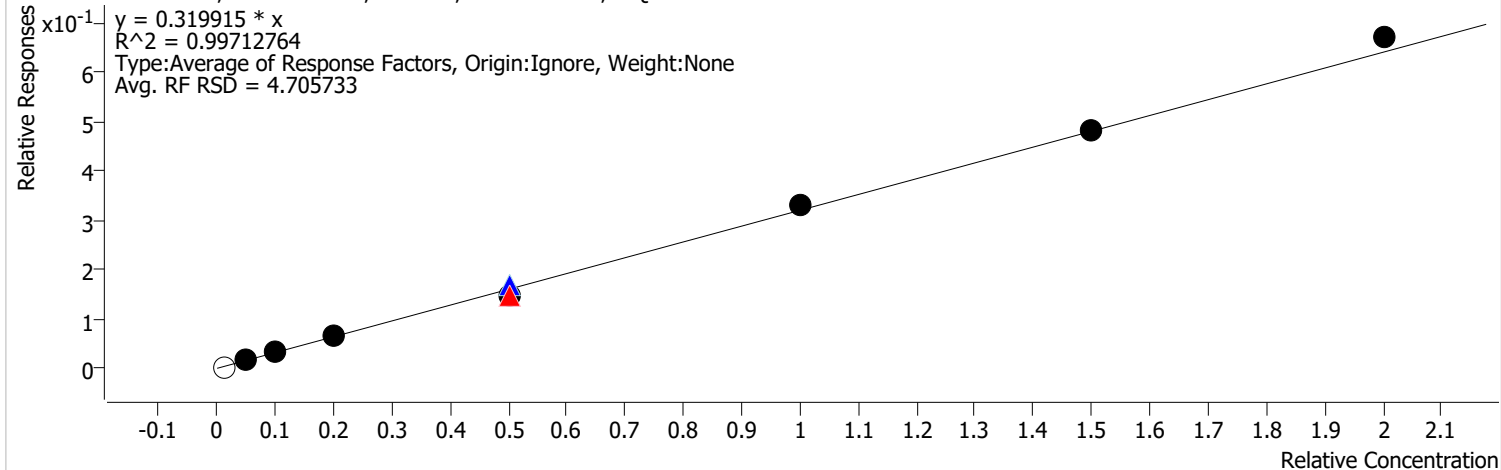


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 708    | 2.5000    | 0.3108       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 3652   | 12.5000   | 0.3016       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 7972   | 25.0000   | 0.3317       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 16073  | 50.0000   | 0.3232       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 42560  | 125.0000  | 0.3326       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 39165  | 125.0000  | 0.2962       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 39165  | 125.0000  | 0.2962       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 87836  | 250.0000  | 0.3295       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 129038 | 375.0000  | 0.3227       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 175918 | 500.0000  | 0.3345       |           |



# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:45 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**p-Bromofluorobenzene %RSE =**

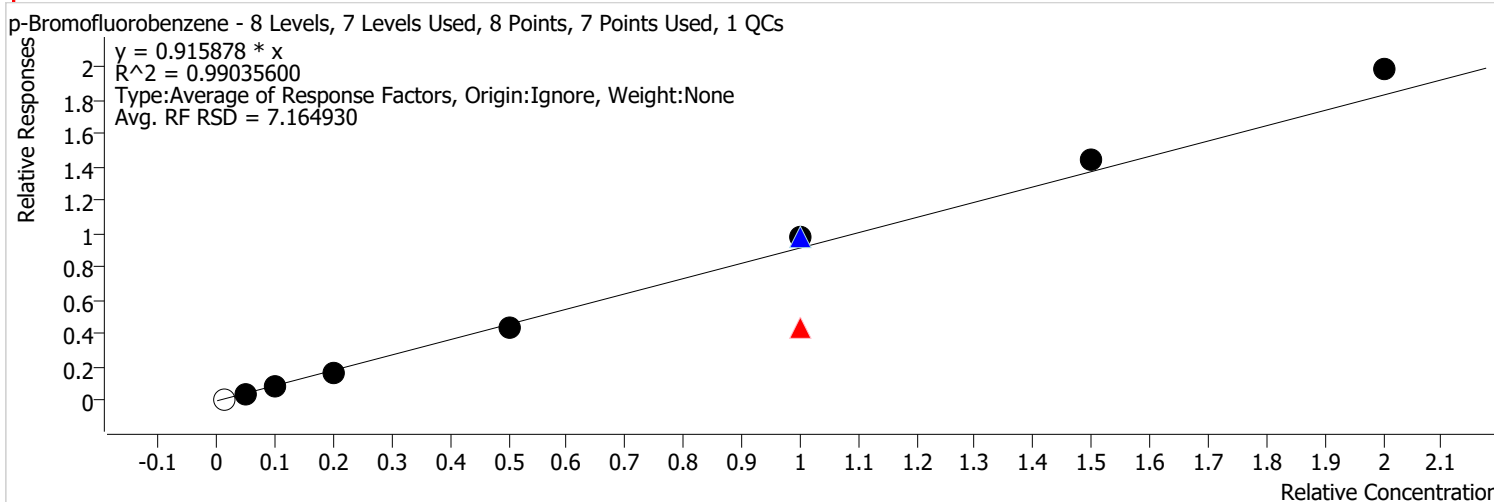


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 2719   | 2.5000    | 1.1932       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 10059  | 12.5000   | 0.8308       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 22267  | 25.0000   | 0.9265       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 42506  | 50.0000   | 0.8548       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 114269 | 125.0000  | 0.8641       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 253034 | 250.0000  | 0.9888       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 261042 | 250.0000  | 0.9793       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 114269 | 250.0000  | 0.4321       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 385474 | 375.0000  | 0.9639       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 521580 | 500.0000  | 0.9917       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:45 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**Bromobenzene %RSE = 3.9**




| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 2024   | 2.5000    | 0.8880       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 9663   | 12.5000   | 0.7981       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 19259  | 25.0000   | 0.8013       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 38282  | 50.0000   | 0.7698       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 109054 | 125.0000  | 0.8523       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 102265 | 125.0000  | 0.7733       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 102265 | 125.0000  | 0.7733       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 227127 | 250.0000  | 0.8521       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 333431 | 375.0000  | 0.8338       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 439147 | 500.0000  | 0.8350       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:45 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**1,1,2,2-Tetrachloroethane %RSE = 5.8**

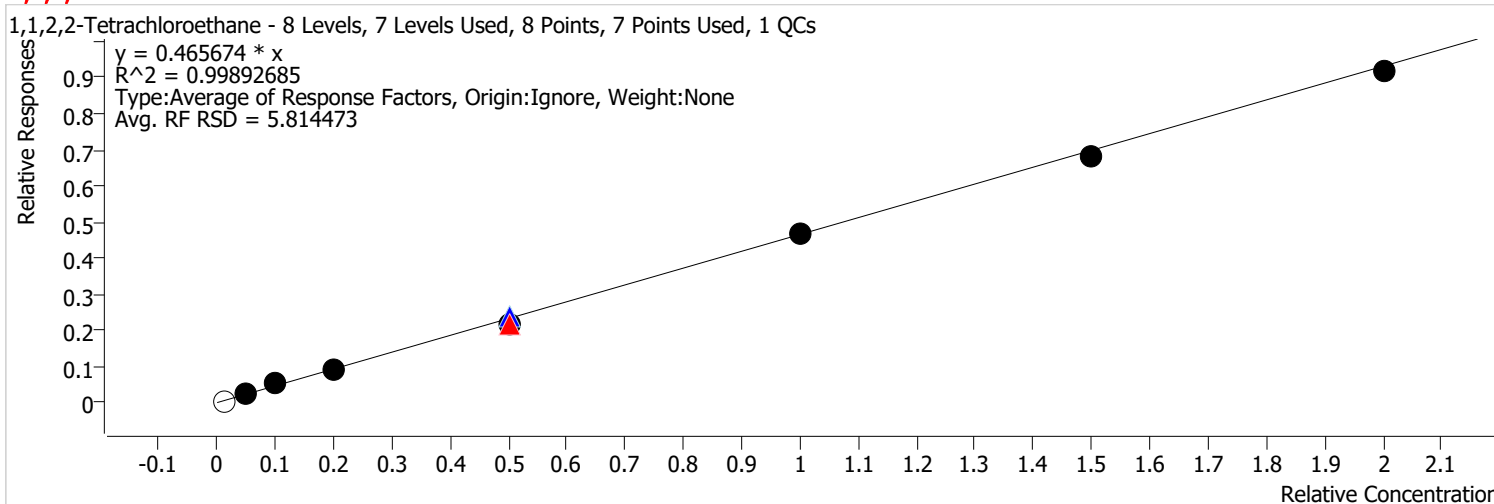


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 1142   | 2.5000    | 0.5014       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 5793   | 12.5000   | 0.4785       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 12440  | 25.0000   | 0.5176       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 22514  | 50.0000   | 0.4528       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 60763  | 125.0000  | 0.4749       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 56958  | 125.0000  | 0.4307       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 56958  | 125.0000  | 0.4307       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 124205 | 250.0000  | 0.4660       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 182470 | 375.0000  | 0.4563       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 240837 | 500.0000  | 0.4579       |           |

# Calibration Report

|                     |                                                                     |                      |                |
|---------------------|---------------------------------------------------------------------|----------------------|----------------|
| Batch Path          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | Analyst Name         | BL2000\mchavez |
| Analysis Time       | 2/28/2022 1:57 PM                                                   | Reporter Name        | BL2000\mchavez |
| Report Time         | 2/28/2022 2:00:45 PM                                                | Batch State          | Processed      |
| Last Calib Update   | 1/9/2022 8:59 PM                                                    | Quant Report Version | 10.0           |
| Quant Batch Version | 10.0                                                                |                      |                |

**1,2,3-Trichloropropane %RSE = 6.5**

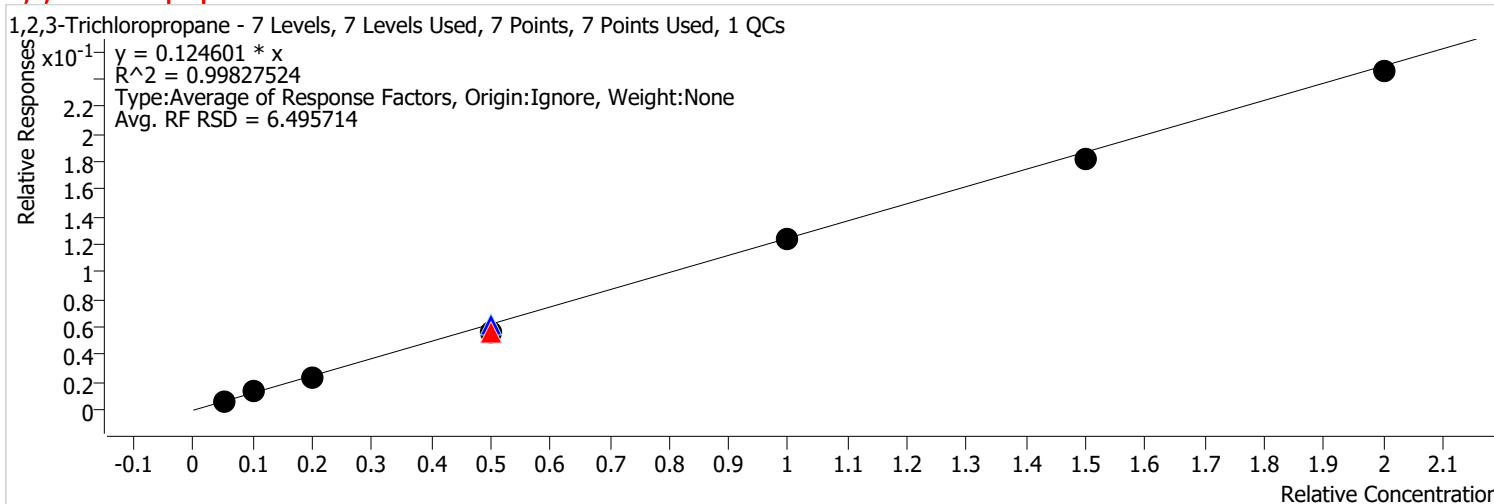


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp. | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|-------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 1654  | 12.5000   | 0.1366       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 3200  | 25.0000   | 0.1331       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 6096  | 50.0000   | 0.1226       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 15682 | 125.0000  | 0.1226       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 14846 | 125.0000  | 0.1123       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 14846 | 125.0000  | 0.1123       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 33115 | 250.0000  | 0.1242       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 48325 | 375.0000  | 0.1208       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 64422 | 500.0000  | 0.1225       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:45 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**2-Chlorotoluene %RSE = 6.8**

2-Chlorotoluene - 8 Levels, 7 Levels Used, 8 Points, 7 Points Used, 1 QCs

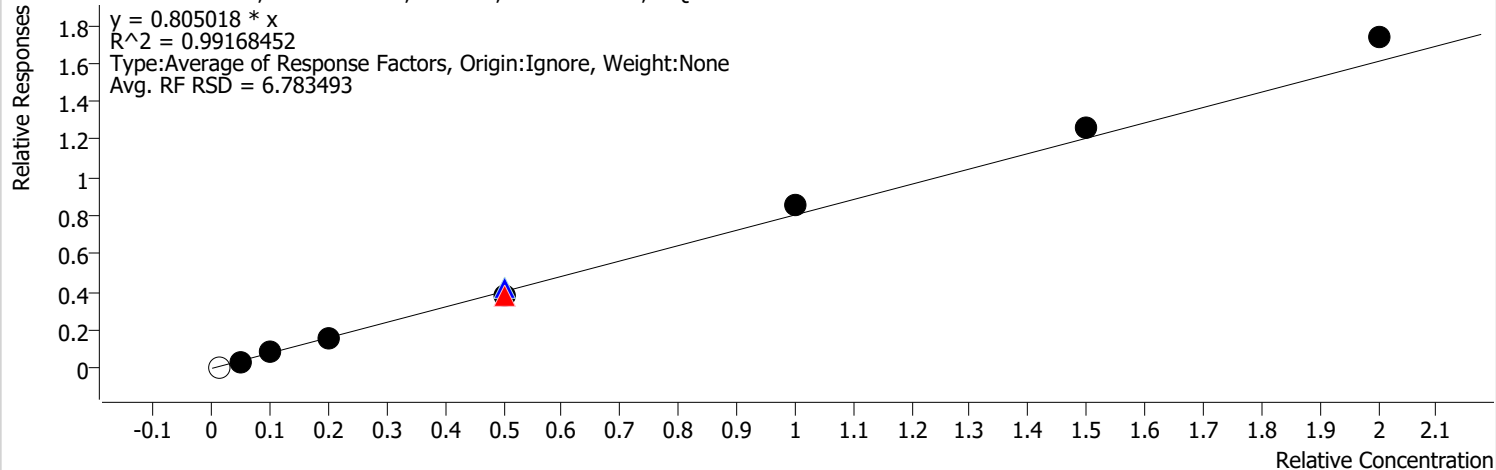


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 1844   | 2.5000    | 0.8090       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 8731   | 12.5000   | 0.7211       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 19390  | 25.0000   | 0.8068       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 37987  | 50.0000   | 0.7639       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 108192 | 125.0000  | 0.8456       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 102424 | 125.0000  | 0.7745       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 102424 | 125.0000  | 0.7745       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 229396 | 250.0000  | 0.8606       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 336386 | 375.0000  | 0.8411       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 455991 | 500.0000  | 0.8670       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:45 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**4-Chlorotoluene %RSE = 6.5**

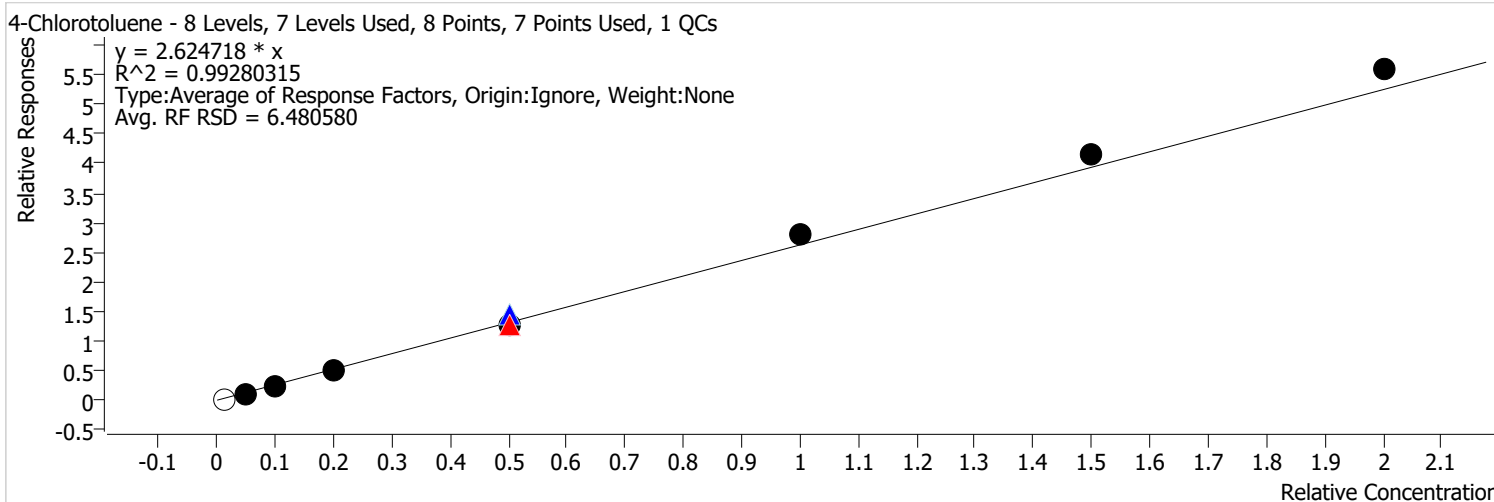


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.   | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|---------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     |         | 5419    | 2.5000    | 2.3780       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 28532   | 12.5000   | 2.3566       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 61551   | 25.0000   | 2.5611       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 126308  | 50.0000   | 2.5400       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 368295  | 125.0000  | 2.8784       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 336146  | 125.0000  | 2.5420       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 336146  | 125.0000  | 2.5420       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 748435  | 250.0000  | 2.8078       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 1109221 | 375.0000  | 2.7736       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 1468376 | 500.0000  | 2.7919       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:45 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**1,3-Dichlorobenzene %RSE = 4.6**

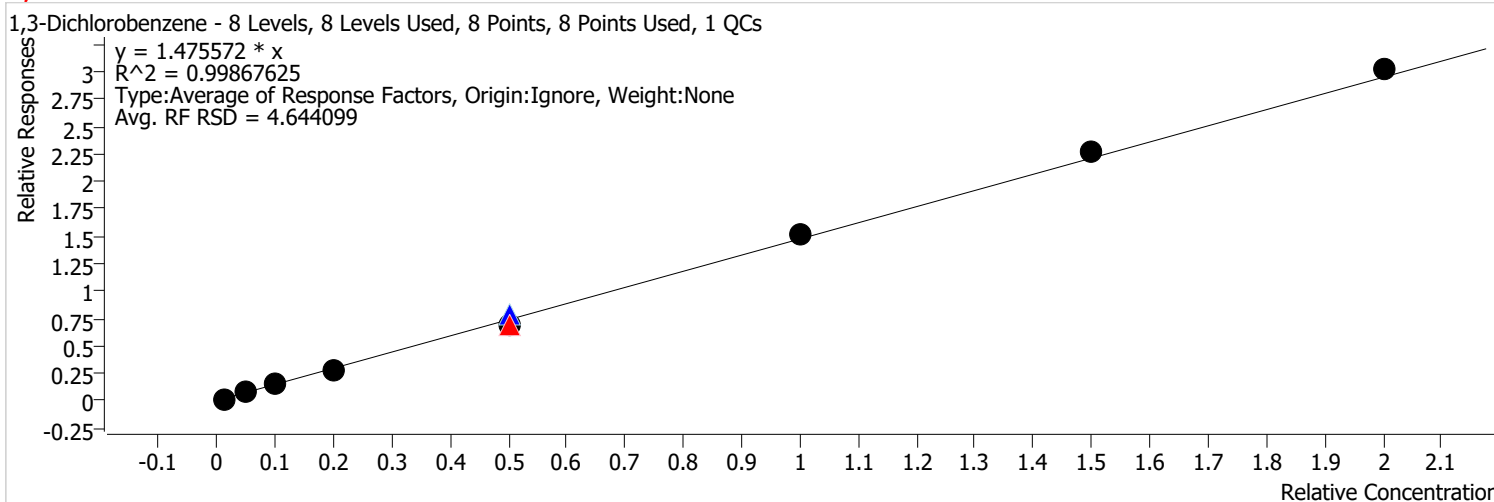


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     | x       | 3541   | 2.5000    | 1.5539       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 16932  | 12.5000   | 1.3985       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 36559  | 25.0000   | 1.5212       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 69539  | 50.0000   | 1.3984       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 204088 | 125.0000  | 1.5950       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 183404 | 125.0000  | 1.3869       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 183404 | 125.0000  | 1.3869       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 406895 | 250.0000  | 1.5265       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 603674 | 375.0000  | 1.5095       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 793993 | 500.0000  | 1.5097       |           |

# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:45 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |

**1,4-Dichlorobenzene %RSE = 5.0**

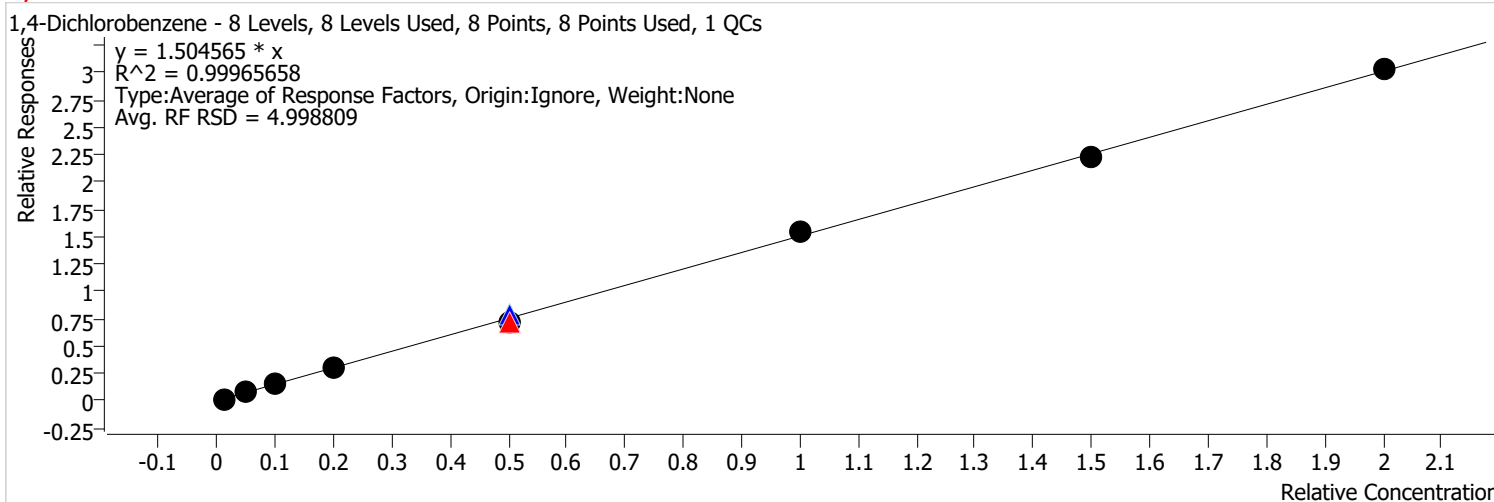


| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     | x       | 3787   | 2.5000    | 1.6618       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 17438  | 12.5000   | 1.4403       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 36635  | 25.0000   | 1.5243       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 71841  | 50.0000   | 1.4447       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 200032 | 125.0000  | 1.5633       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 189045 | 125.0000  | 1.4296       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 189045 | 125.0000  | 1.4296       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 408934 | 250.0000  | 1.5342       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 595919 | 375.0000  | 1.4901       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 794954 | 500.0000  | 1.5115       |           |



# Calibration Report

|                            |                                                                     |                             |                |
|----------------------------|---------------------------------------------------------------------|-----------------------------|----------------|
| <b>Batch Path</b>          | D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin | <b>Analyst Name</b>         | BL2000\mchavez |
| <b>Analysis Time</b>       | 2/28/2022 1:57 PM                                                   | <b>Reporter Name</b>        | BL2000\mchavez |
| <b>Report Time</b>         | 2/28/2022 2:00:45 PM                                                | <b>Batch State</b>          | Processed      |
| <b>Last Calib Update</b>   | 1/9/2022 8:59 PM                                                    | <b>Quant Report Version</b> | 10.0           |
| <b>Quant Batch Version</b> | 10.0                                                                |                             |                |


**1,2-Dichlorobenzene %RSE = 4.9**

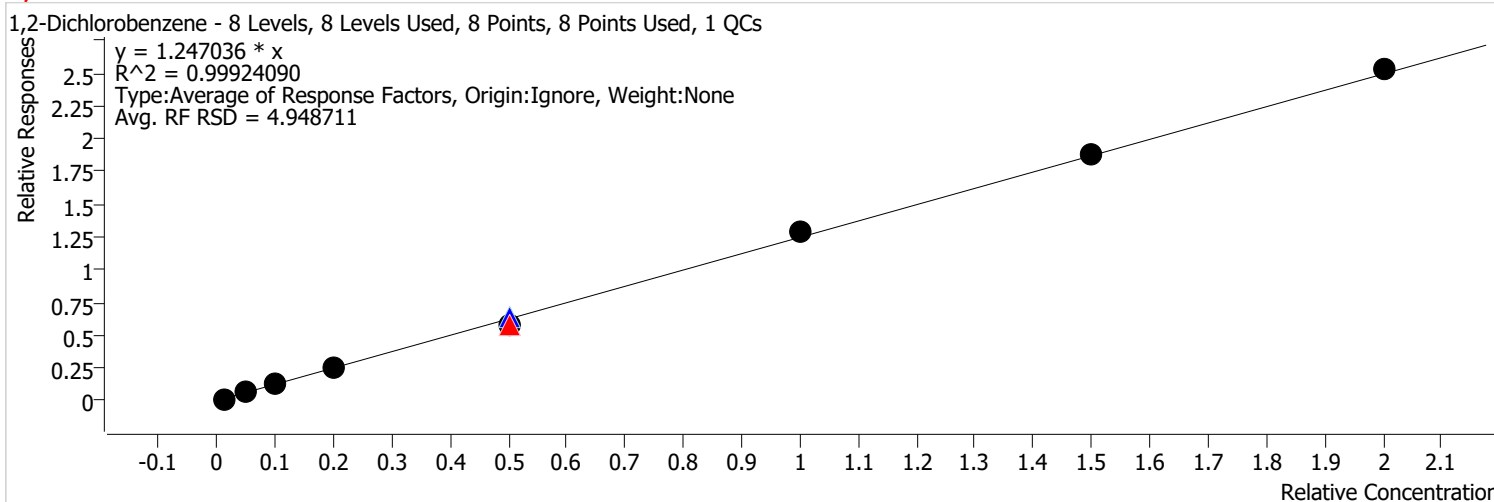

| Calibration STD Path                      | Cal Type    | Level | Enabled | Resp.  | Exp. Conc | Resp. Factor | Level RSD |
|-------------------------------------------|-------------|-------|---------|--------|-----------|--------------|-----------|
| D:\Org\Data\VOA5975C\VG010422\04JAN10.D   | Calibration | 1     | x       | 3104   | 2.5000    | 1.3621       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN11.D   | Calibration | 2     | x       | 14666  | 12.5000   | 1.2114       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN12.D   | Calibration | 3     | x       | 29899  | 25.0000   | 1.2441       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN13.D   | Calibration | 4     | x       | 60213  | 50.0000   | 1.2109       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN23.D   | QC          | QC    | x       | 164299 | 125.0000  | 1.2841       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15.D   | Calibration | 5     | x       | 152284 | 125.0000  | 1.1516       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D | CC          | CC    | x       | 152284 | 125.0000  | 1.1516       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN17.D   | Calibration | 6     | x       | 342576 | 250.0000  | 1.2852       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN19.D   | Calibration | 7     | x       | 499147 | 375.0000  | 1.2481       |           |
| D:\Org\Data\VOA5975C\VG010422\04JAN21.D   | Calibration | 8     | x       | 664247 | 500.0000  | 1.2630       |           |

# Quantitation Results Report (QT Reviewed)

|                |                                     |                   |                       |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File      | 04JAN09.D                           | Operator          | MSC                   |
| Acq. Method    | 5975CACQF.M                         | Acq. Date-Time    | 1/4/2022 3:05:37 PM   |
| Sample Name    | MBLK010422_                         | Instrument        | VOA5975C              |
| Vial           | 9                                   | Multiplier        | 1.00                  |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m  | Comment           |                       |
| Tune File      | BFB_Atune3.u                        | Tune Date         | 10/11/2021 4:02:00 PM |
| Batch Name     | VG010422_8260B.batch.bin            | Last Calib Update | 1/9/2022 8:59:52 PM   |
| Ref Library    | \\MASSHUNTER\Org\Library\NIST129K.I |                   |                       |

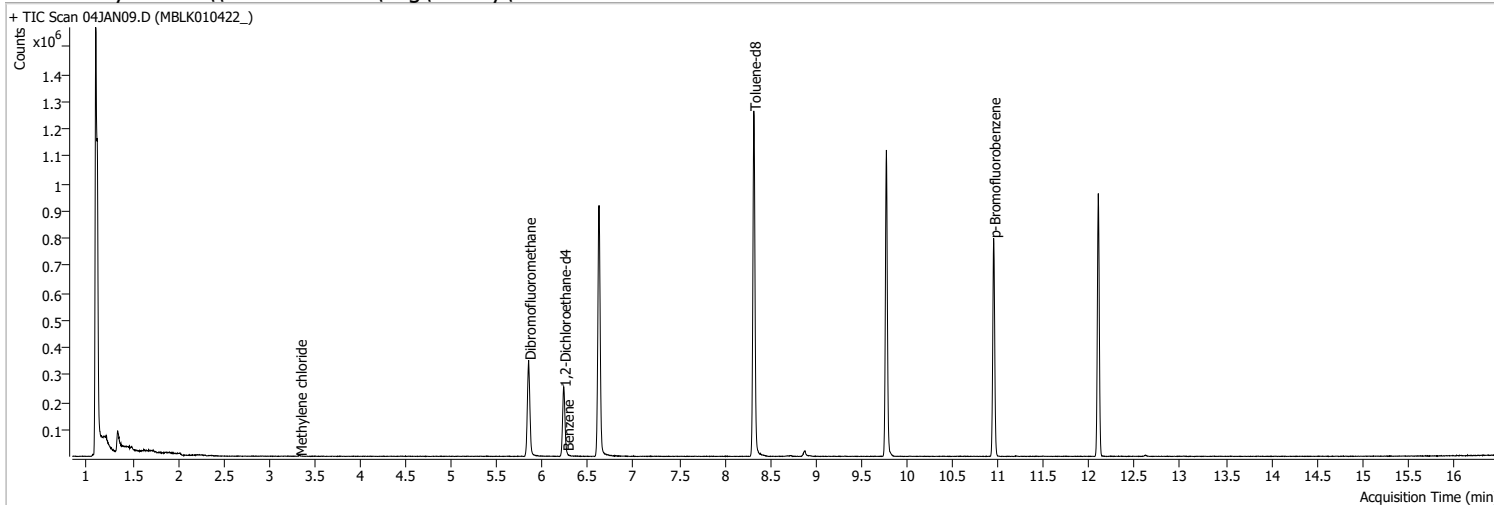









| Compound                           | RT                   | QIon  | Resp.  | Conc.              | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|--------------------|-------|----------|
| <b>Internal Standards</b>          |                      |       |        |                    |       |          |
| M Fluorobenzene                    | 6.620                | 96.0  | 775552 | 250.0000           | ng    | -0.003   |
| M Chlorobenzene-d5                 | 9.774                | 82.0  | 301196 | 250.0000           | ng    | 0.003    |
| M 1,4-Dichlorobenzene-d4           | 12.100               | 152.0 | 231562 | 250.0000           | ng    | 0.000    |
| <b>System Monitoring Compounds</b> |                      |       |        |                    |       |          |
| S Dibromofluoromethane             | 5.848                | 113.0 | 203459 | 278.4635           | ng    | 0.003    |
| Spiked Amount: 250.000             | Range: 80.0 - 119.0% |       |        | Recovery = 111.39% |       |          |
| S 1,2-Dichloroethane-d4            | 6.233                | 67.0  | 88174  | 279.3964           | ng    | 0.000    |
| Spiked Amount: 250.000             | Range: 81.0 - 118.0% |       |        | Recovery = 111.76% |       |          |
| S Toluene-d8                       | 8.319                | 98.0  | 770154 | 265.3436           | ng    | 0.000    |
| Spiked Amount: 250.000             | Range: 89.0 - 112.0% |       |        | Recovery = 106.14% |       |          |
| S p-Bromofluorobenzene             | 10.951               | 95.0  | 226743 | 267.2815           | ng    | -0.003   |
| Spiked Amount: 250.000             | Range: 85.0 - 114.0% |       |        | Recovery = 106.91% |       |          |
| <b>Target Compounds</b>            |                      |       |        |                    |       |          |
| T Dichlorodifluoromethane          | 0.000                |       | 0      | N.D.               |       |          |
| T Chloromethane                    | 1.333                | 50.0  | 0      |                    | ng    | md 1     |
| T Vinyl chloride                   | 1.489                | 62.0  | 0      |                    | ng    | md 1     |
| T Bromomethane                     | 0.000                |       | 0      | N.D.               |       |          |
| T Chloroethane                     | 0.000                |       | 0      | N.D.               |       |          |
| T Trichlorofluoromethane           | 0.000                |       | 0      | N.D.               |       |          |
| T 1,1-Dichloroethene               | 0.000                |       | 0      | N.D.               |       |          |
| T Methylene chloride               | 3.335                | 49.0  | 1661   | 1.4424             | ng    | m 97     |
| T trans-1,2-Dichloroethene         | 0.000                |       | 0      | N.D.               |       |          |
| T Methyl tert-butyl ether (MTBE)   | 0.000                |       | 0      | N.D.               |       |          |
| T 1,1-Dichloroethane               | 0.000                |       | 0      | N.D.               |       |          |
| T 2,2-Dichloropropane              | 0.000                |       | 0      | N.D.               |       |          |
| T cis-1,2-Dichloroethene           | 0.000                |       | 0      | N.D.               |       |          |
| T Methyl ethyl ketone              | 0.000                |       | 0      | N.D.               |       |          |
| T Bromochloromethane               | 0.000                |       | 0      | N.D.               |       |          |
| T Chloroform                       | 0.000                |       | 0      | N.D.               |       |          |

# Quantitation Results Report (QT Reviewed)

| Compound                    | RT    | QIon | Resp. | Conc.  | Units |   | Dev(Min) |
|-----------------------------|-------|------|-------|--------|-------|---|----------|
| T 1,1,1-Trichloroethane     | 0.000 |      | 0     | N.D.   |       |   |          |
| T Carbon tetrachloride      | 0.000 |      | 0     | N.D.   |       |   |          |
| T 1,1-Dichloropropene       | 0.000 |      | 0     | N.D.   |       |   |          |
| T Benzene                   | 6.266 | 78.0 | 381   | 0.1233 | ng    | m | 98       |
| T 1,2-Dichloroethane        | 0.000 |      | 0     | N.D.   |       |   |          |
| T Trichloroethene           | 0.000 |      | 0     | N.D.   |       |   |          |
| T 1,2-Dichloropropane       | 0.000 |      | 0     | N.D.   |       |   |          |
| T Dibromomethane            | 0.000 |      | 0     | N.D.   |       |   |          |
| T Bromodichloromethane      | 0.000 |      | 0     | N.D.   |       |   |          |
| T cis-1,3-Dichloropropene   | 0.000 |      | 0     | N.D.   |       |   |          |
| T Toluene                   | 0.000 |      | 0     | N.D.   |       |   |          |
| T trans-1,3-Dichloropropene | 0.000 |      | 0     | N.D.   |       |   |          |
| T 1,1,2-Trichloroethane     | 0.000 |      | 0     | N.D.   |       |   |          |
| T Tetrachloroethene         | 0.000 |      | 0     | N.D.   |       |   |          |
| T 1,3-Dichloropropane       | 0.000 |      | 0     | N.D.   |       |   |          |
| T Chlorodibromomethane      | 0.000 |      | 0     | N.D.   |       |   |          |
| T 1,2-Dibromoethane         | 0.000 |      | 0     | N.D.   |       |   |          |
| T Chlorobenzene             | 0.000 |      | 0     | N.D.   |       |   |          |
| T 1,1,1,2-Tetrachloroethane | 0.000 |      | 0     | N.D.   |       |   |          |
| T Ethylbenzene              | 0.000 |      | 0     | N.D.   |       |   |          |
| T m+p-Xylenes               | 0.000 |      | 0     | N.D.   |       |   |          |
| T o-Xylene                  | 0.000 |      | 0     | N.D.   |       |   |          |
| T Styrene                   | 0.000 |      | 0     | N.D.   |       |   |          |
| T Bromoform                 | 0.000 |      | 0     | N.D.   |       |   |          |
| T Bromobenzene              | 0.000 |      | 0     | N.D.   |       |   |          |
| T 1,1,2,2-Tetrachloroethane | 0.000 |      | 0     | N.D.   |       |   |          |
| T 1,2,3-Trichloropropane    | 0.000 |      | 0     | N.D.   |       |   |          |
| T 2-Chlorotoluene           | 0.000 |      | 0     | N.D.   |       |   |          |
| T 4-Chlorotoluene           | 0.000 |      | 0     | N.D.   |       |   |          |
| T 1,3-Dichlorobenzene       | 0.000 |      | 0     | N.D.   |       |   |          |
| T 1,4-Dichlorobenzene       | 0.000 |      | 0     | N.D.   |       |   |          |
| T 1,2-Dichlorobenzene       | 0.000 |      | 0     | N.D.   |       |   |          |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (\*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

# Quantitation Results Report (QT Reviewed)

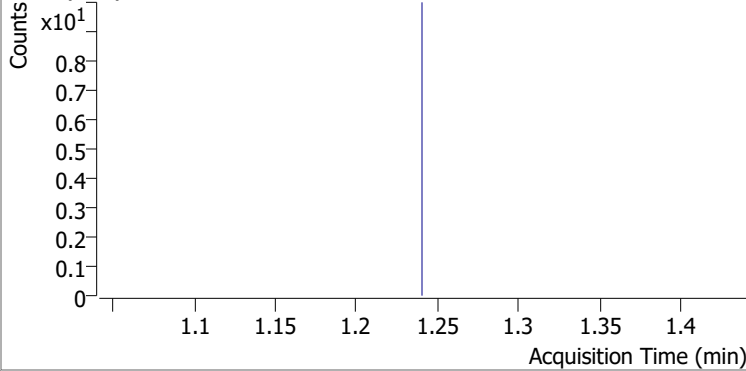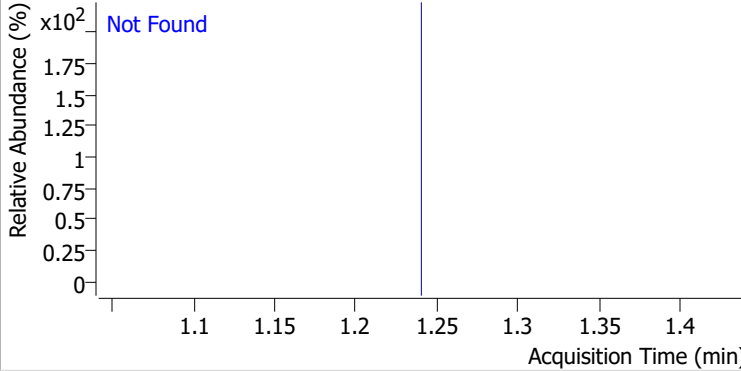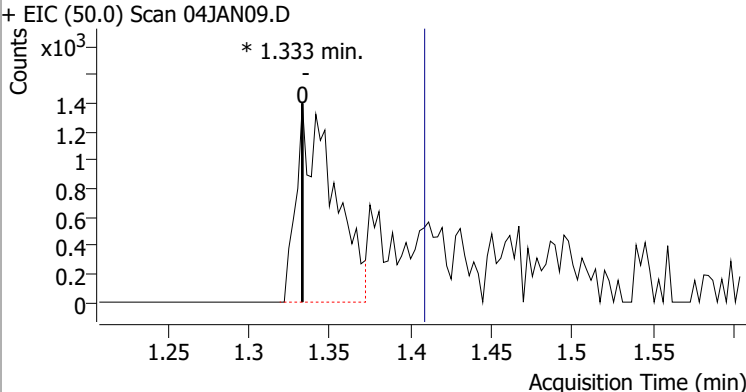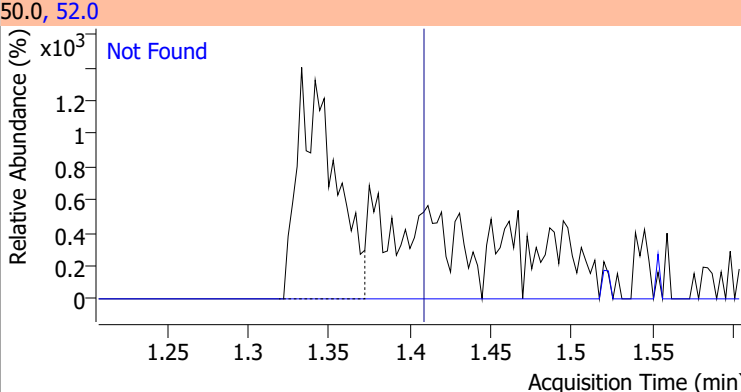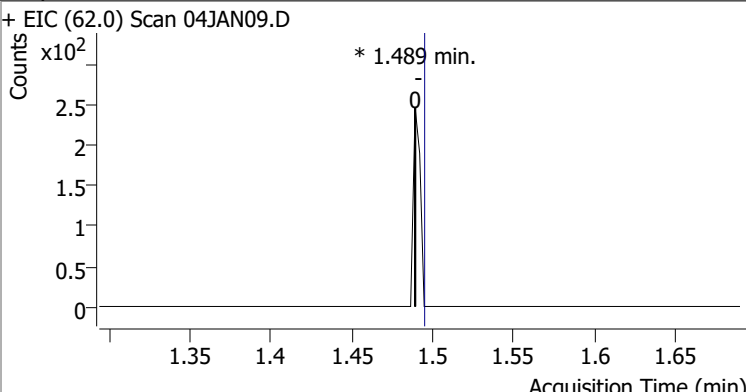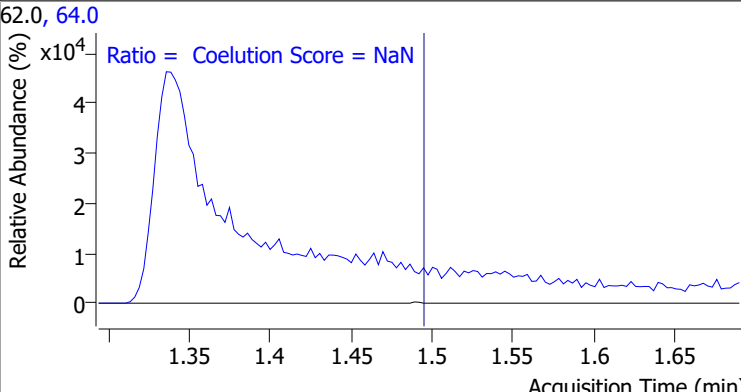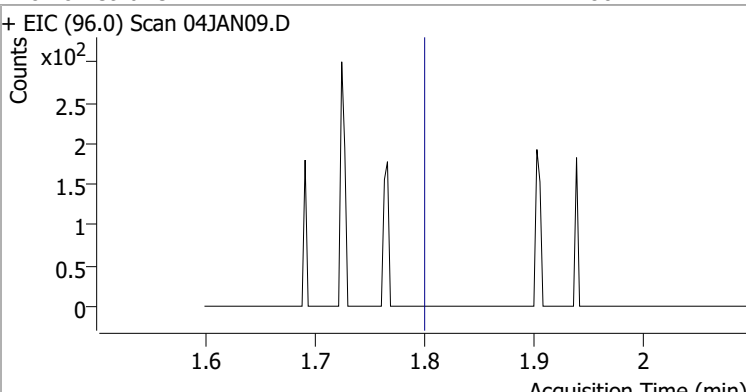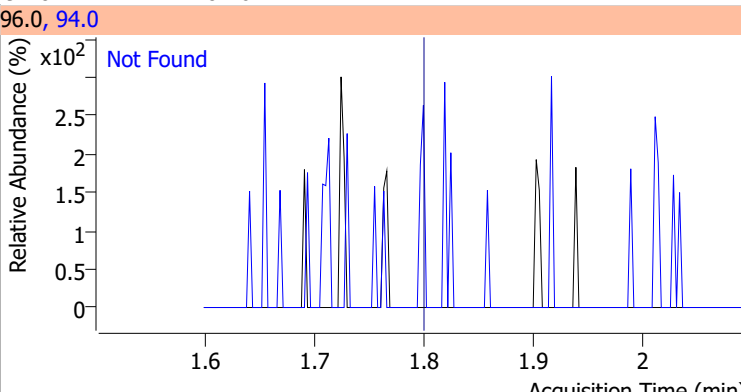
| Compound                                                                           | Conc. | Exp RT | QIon                                                                                                                                           | Exp Ratio |      |        |       |       |
|------------------------------------------------------------------------------------|-------|--------|------------------------------------------------------------------------------------------------------------------------------------------------|-----------|------|--------|-------|-------|
| Dichlorodifluoromethane                                                            | N.D.  | 1.24   | 87.0                                                                                                                                           | 32.3      |      |        |       |       |
| + EIC (85.0) Scan 04JAN09.D ***NO DATA POINTS***                                   |       |        | 85.0, 87.0                                                                                                                                     |           |      |        |       |       |
|    |       |        |  <p style="color: blue;">Not Found</p>                       |           |      |        |       |       |
| Compound                                                                           | Conc. | RT     | Dev(Min)                                                                                                                                       | Resp.     | QIon | QRatio | Lower | Upper |
| Chloromethane                                                                      | 0     | 0      | 0                                                                                                                                              | 0         | 52.0 |        | 2.1   | 62.1  |
| + EIC (50.0) Scan 04JAN09.D                                                        |       |        | 50.0, 52.0                                                                                                                                     |           |      |        |       |       |
|   |       |        |  <p style="color: blue;">Not Found</p>                      |           |      |        |       |       |
| Compound                                                                           | Conc. | RT     | Dev(Min)                                                                                                                                       | Resp.     | QIon | QRatio | Lower | Upper |
| Vinyl chloride                                                                     | 0     | 0      | 0                                                                                                                                              | 0         | 64.0 |        | 0.0   | 59.9  |
| + EIC (62.0) Scan 04JAN09.D                                                        |       |        | 62.0, 64.0                                                                                                                                     |           |      |        |       |       |
|  |       |        |  <p style="color: blue;">Ratio = Coelution Score = NaN</p> |           |      |        |       |       |
| Compound                                                                           | Conc. | Exp RT | QIon                                                                                                                                           | Exp Ratio |      |        |       |       |
| Bromomethane                                                                       | N.D.  | 1.80   | 94.0                                                                                                                                           | 104.6     |      |        |       |       |
| + EIC (96.0) Scan 04JAN09.D                                                        |       |        | 96.0, 94.0                                                                                                                                     |           |      |        |       |       |
|  |       |        |  <p style="color: blue;">Not Found</p>                     |           |      |        |       |       |

# Quantitation Results Report (QT Reviewed)


| Compound     | Conc. | Exp RT | QIon | Exp Ratio |
|--------------|-------|--------|------|-----------|
| Chloroethane | N.D.  | 1.89   | 66.0 | 30.1      |




| Compound               | Conc. | Exp RT | QIon  | Exp Ratio |
|------------------------|-------|--------|-------|-----------|
| Trichlorofluoromethane | N.D.  | 2.14   | 103.0 | 64.2      |



| Compound           | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethene | N.D.  | 2.70   | 61.0 | 180.3     | 63.0 | 56.7      |




| Compound           | Conc.  | RT   | Dev(Min) | Resp.    | QIon | QRatio | Lower | Upper |
|--------------------|--------|------|----------|----------|------|--------|-------|-------|
| Methylene chloride | 1.4424 | 3.34 | 0.00     | 1661 (m) | 84.0 | 64.7   | 36.9  | 96.9  |
|                    |        |      |          |          | 86.0 | 41.8   | 14.3  | 74.3  |




# Quantitation Results Report (QT Reviewed)


| Compound                 | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,2-Dichloroethene | N.D.  | 3.72   | 61.0 | 153.9     | 98.0 | 65.7      |




| Compound                       | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------------------|-------|--------|------|-----------|
| Methyl tert-butyl ether (MTBE) | N.D.  | 3.75   | 57.0 | 24.6      |



| Compound           | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethane | N.D.  | 4.38   | 65.0 | 32.1      | 83.0 | 13.7      |




| Compound            | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|------|-----------|
| 2,2-Dichloropropane | N.D.  | 5.20   | 41.0 | 66.5      | 97.0 | 23.2      |




# Quantitation Results Report (QT Reviewed)


| Compound               | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|------------------------|-------|--------|------|-----------|------|-----------|
| cis-1,2-Dichloroethene | N.D.  | 5.22   | 61.0 | 167.2     | 98.0 | 67.3      |

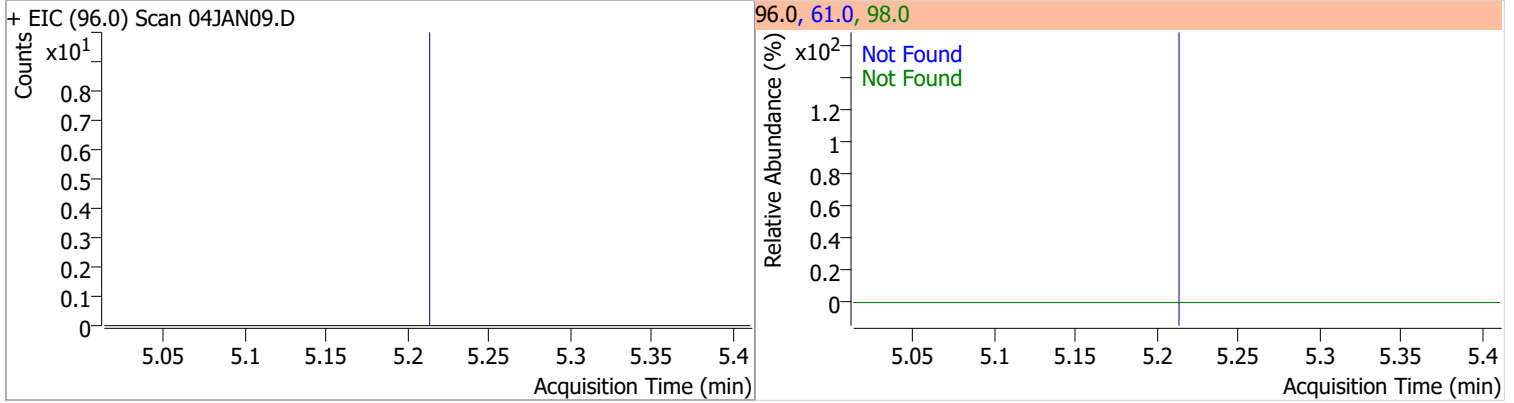


| Compound            | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| Methyl ethyl ketone | N.D.  | 5.28   | 72.0 | 21.3      |

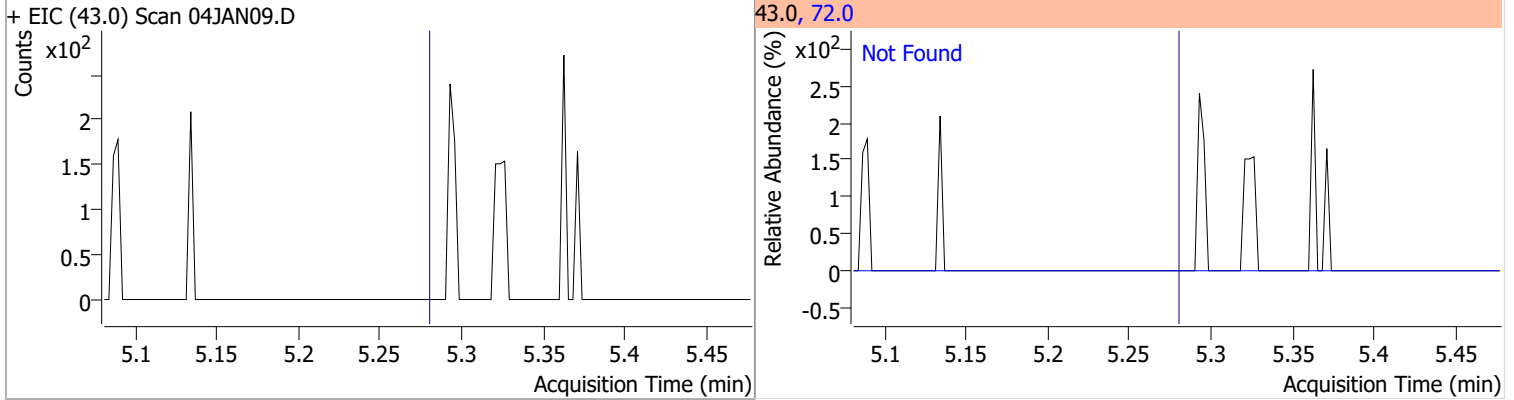





| Compound           | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|
| Bromochloromethane | N.D.  | 5.52   | 49.0 | 182.9     |

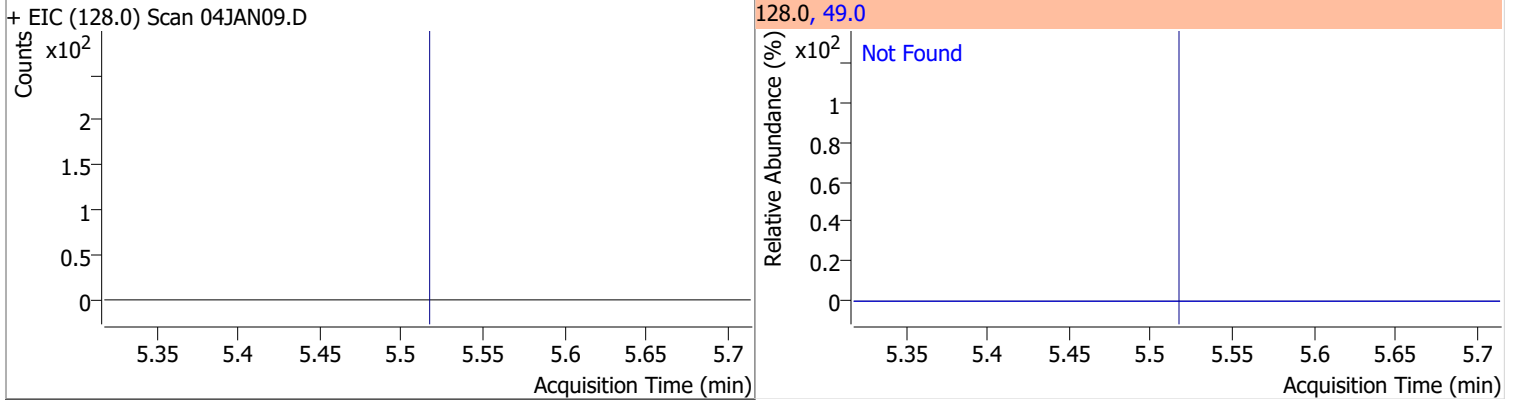

| Compound   | Conc. | Exp RT | QIon | Exp Ratio |
|------------|-------|--------|------|-----------|
| Chloroform | N.D.  | 5.65   | 85.0 | 66.0      |

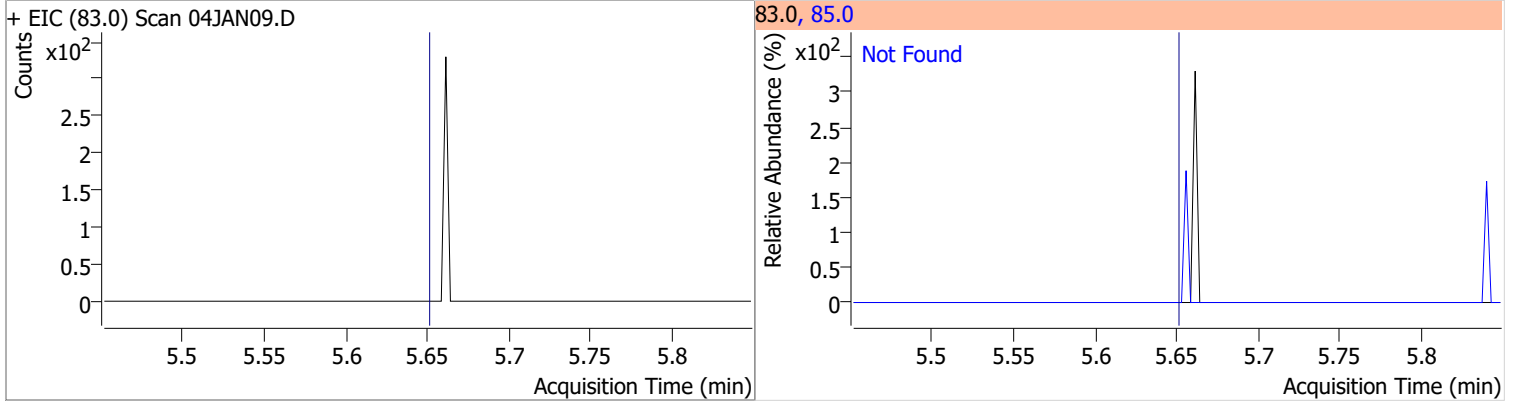


# Quantitation Results Report (QT Reviewed)






# Quantitation Results Report (QT Reviewed)


| Compound              | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 279.3964 | 6.23 | 0.00     | 88174 | 65.0 | 198.1  | 166.5 | 226.5 |

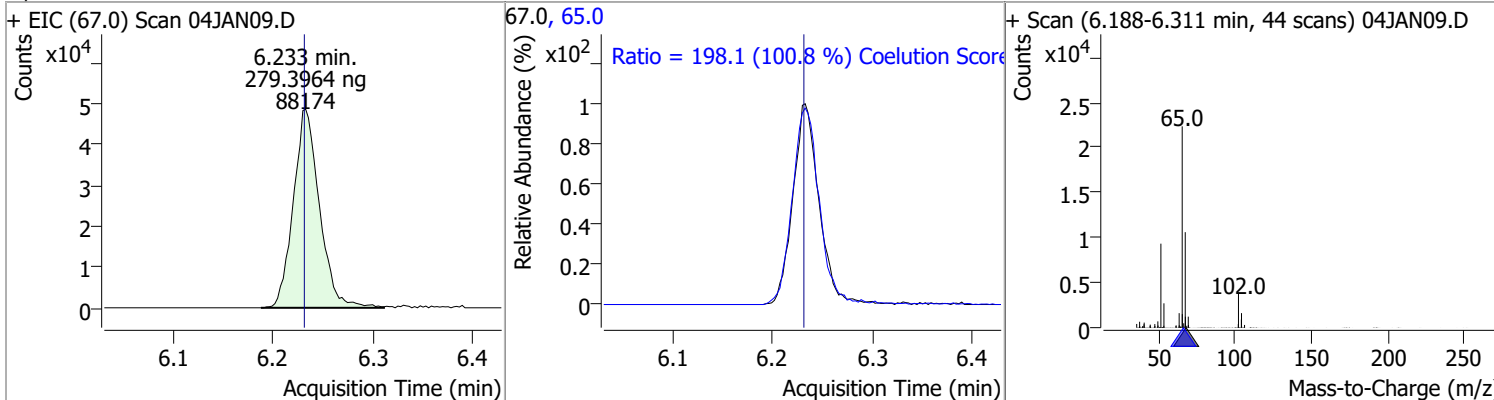


| Compound | Conc.  | RT   | Dev(Min) | Resp.   | QIon | QRatio | Lower | Upper |
|----------|--------|------|----------|---------|------|--------|-------|-------|
| Benzene  | 0.1233 | 6.27 | -0.01    | 381 (m) | 77.0 | 22.7   | 0.0   | 53.5  |

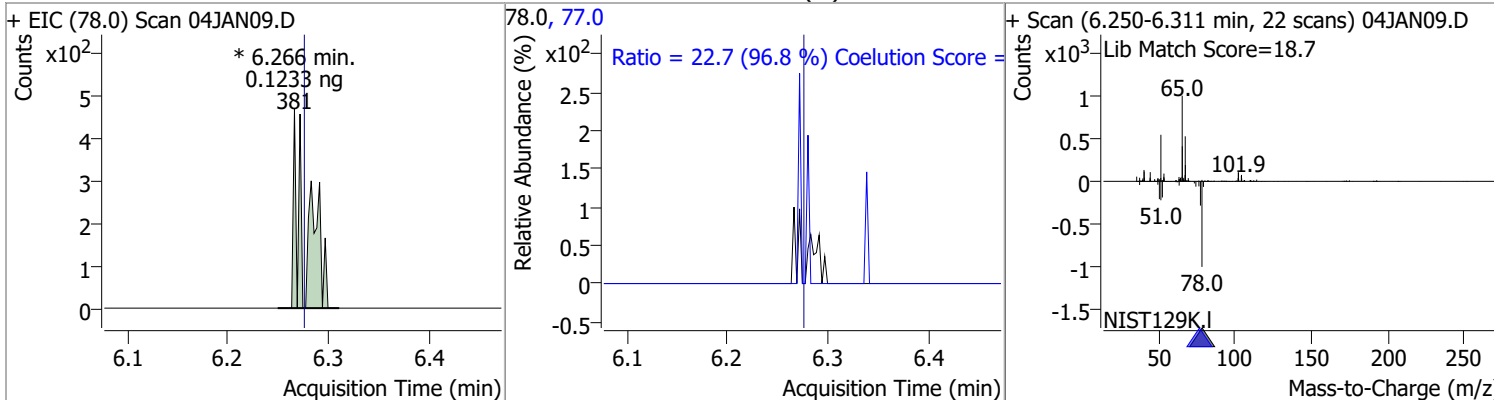





| Compound           | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,2-Dichloroethane | N.D.  | 6.32   | 64.0 | 29.9      | 98.0 | 7.6       |

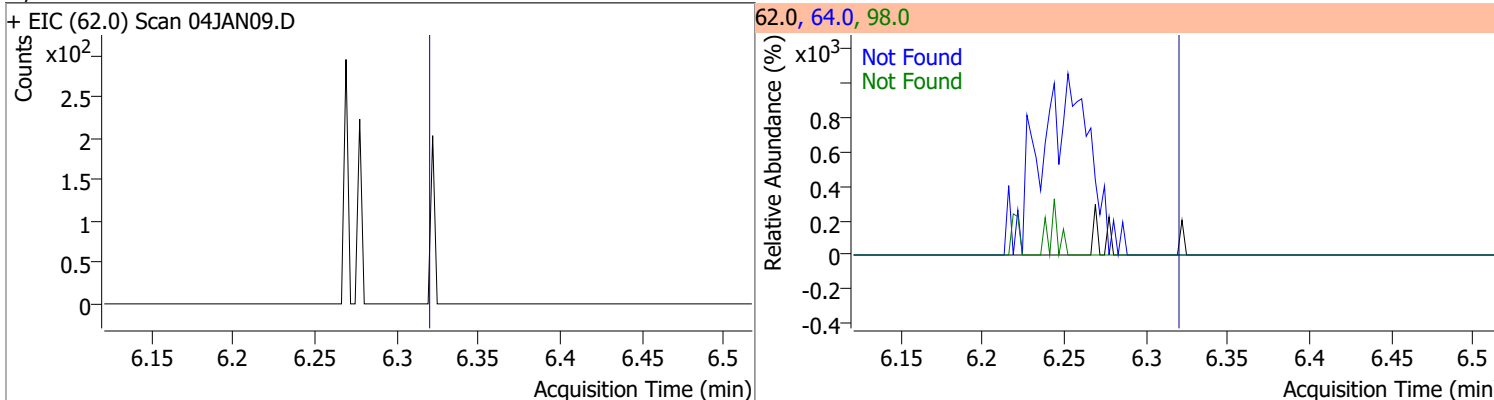

| Compound        | Conc. | Exp RT | QIon  | Exp Ratio | QIon | Exp Ratio |
|-----------------|-------|--------|-------|-----------|------|-----------|
| Trichloroethene | N.D.  | 7.03   | 130.0 | 101.5     | 97.0 | 64.1      |

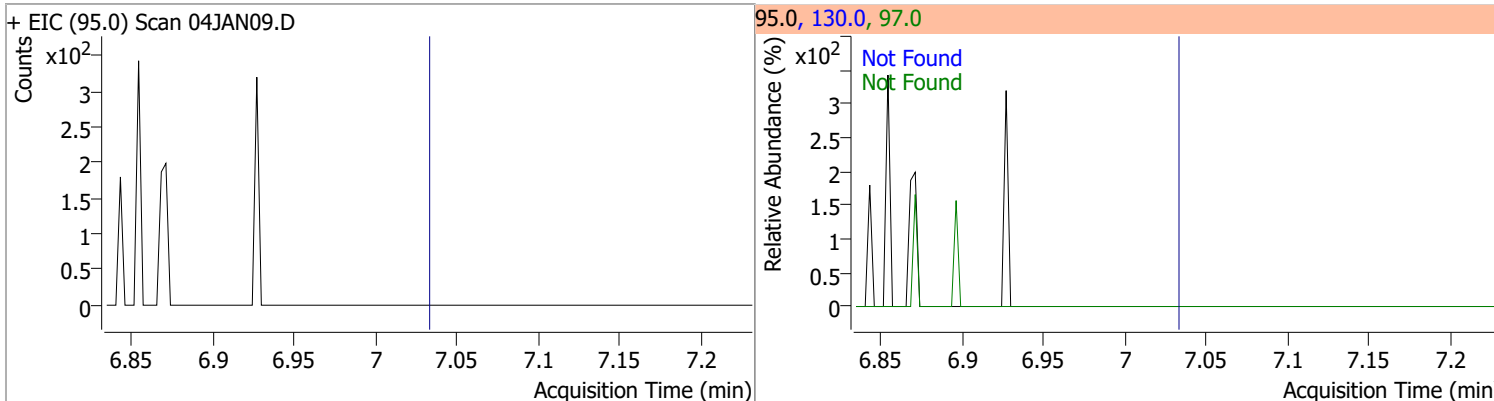


# Quantitation Results Report (QT Reviewed)

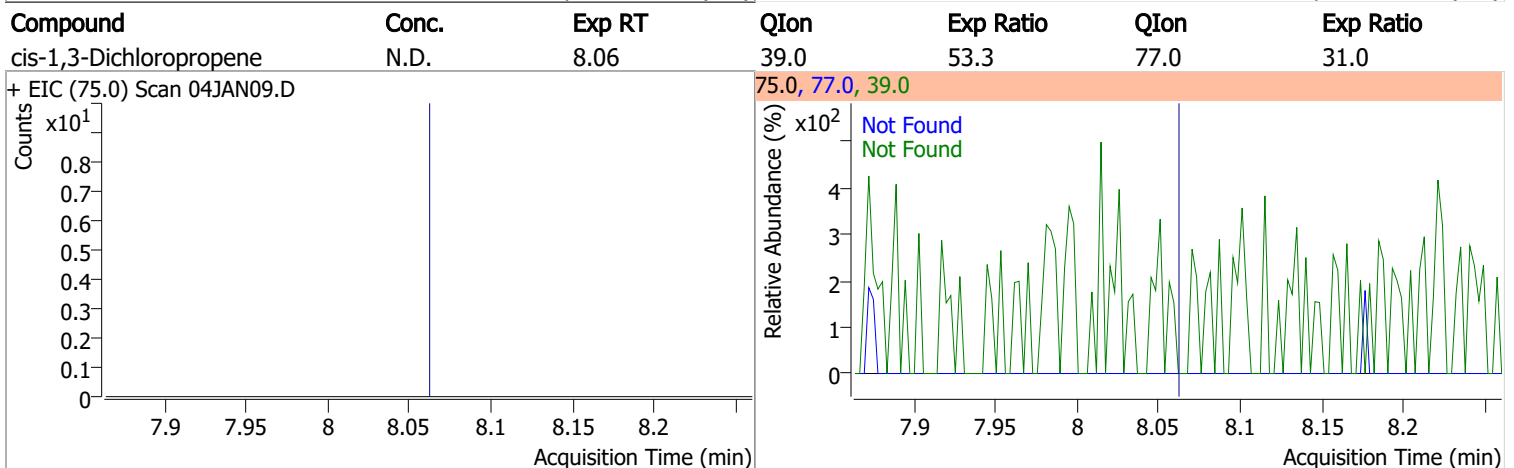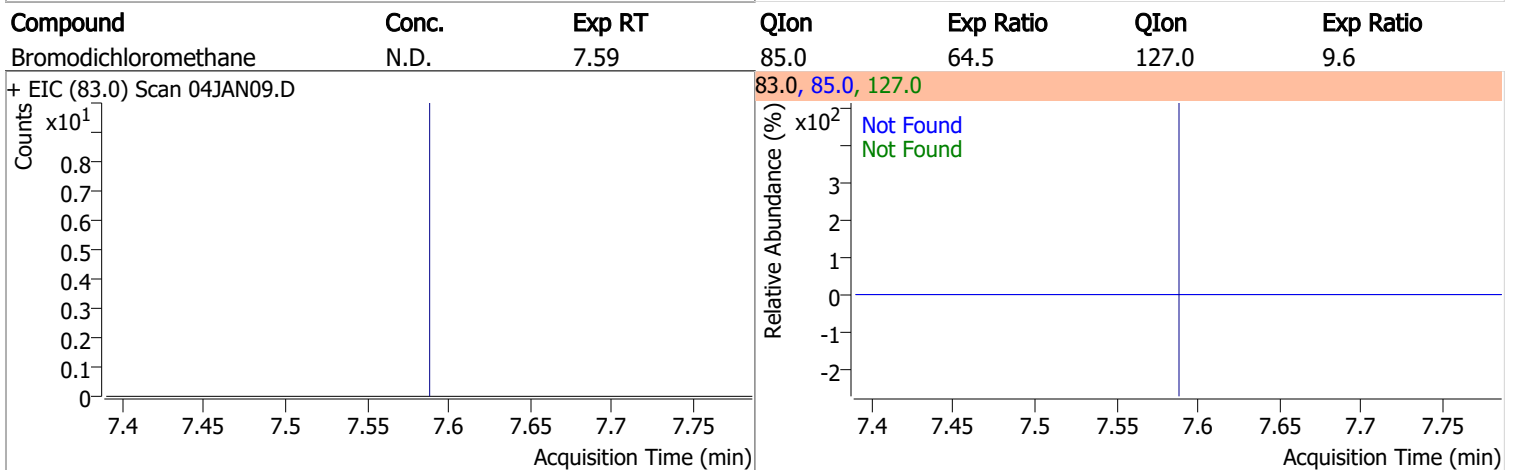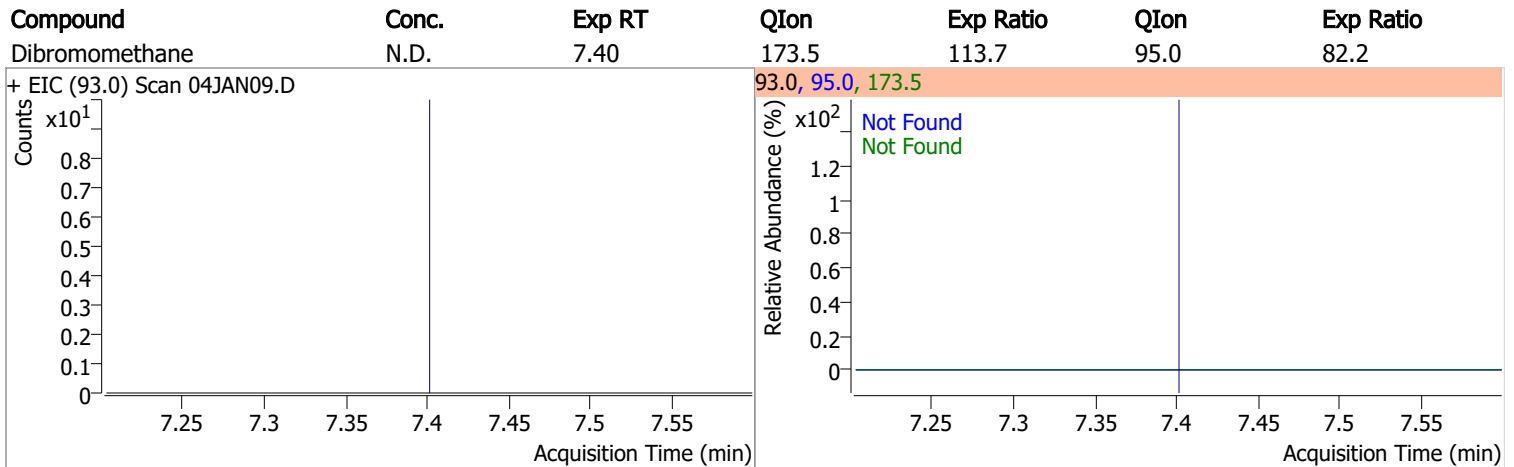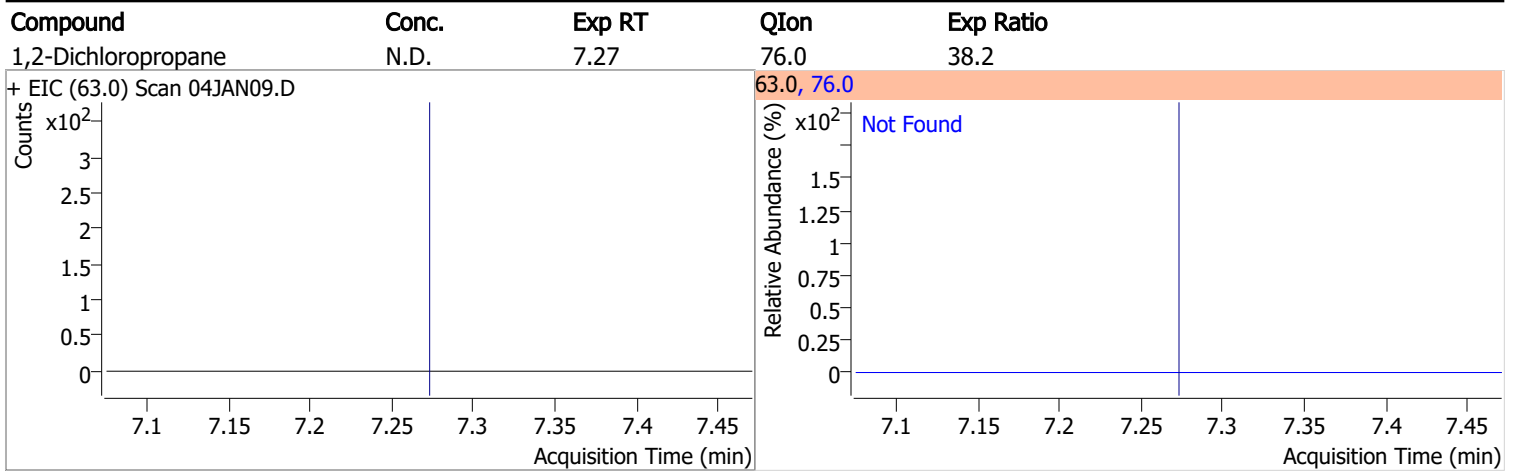


# Quantitation Results Report (QT Reviewed)


| Compound   | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 265.3436 | 8.32 | 0.00     | 770154 | 100.0 | 64.0   | 34.4  | 94.4  |
|            |          |      |          |        | 99.0  | 9.8    | 0.0   | 39.6  |

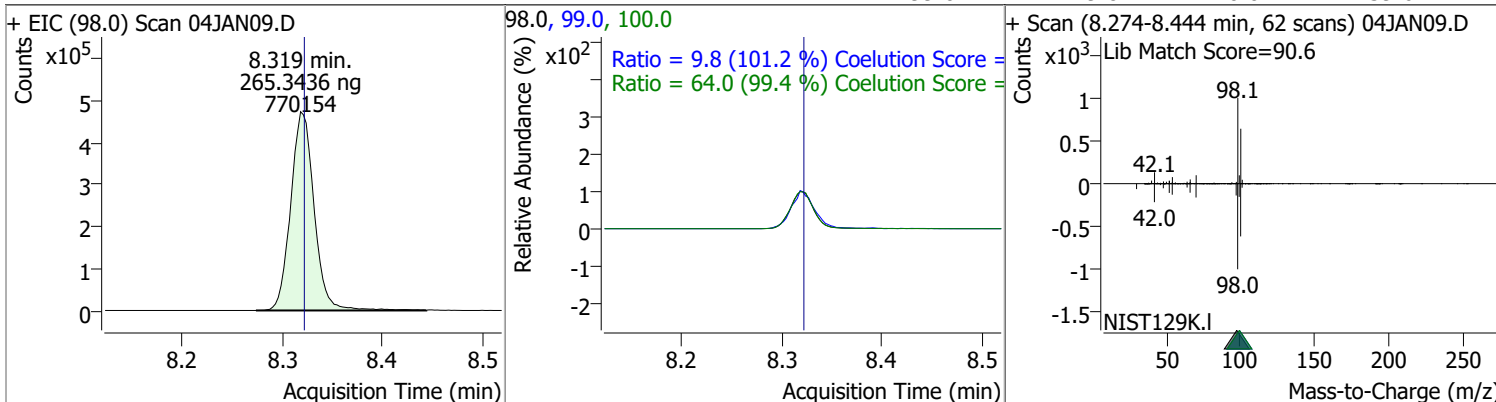


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------|-------|--------|------|-----------|
| Toluene  | N.D.  | 8.39   | 91.0 | 175.8     |

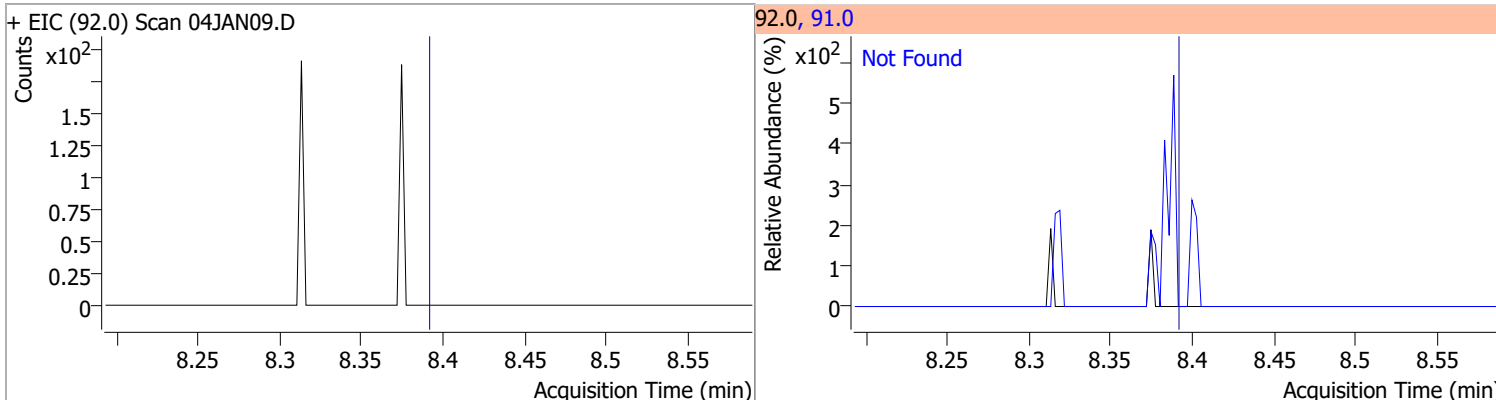









| Compound                  | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,3-Dichloropropene | N.D.  | 8.64   | 39.0 | 53.4      | 77.0 | 32.4      |

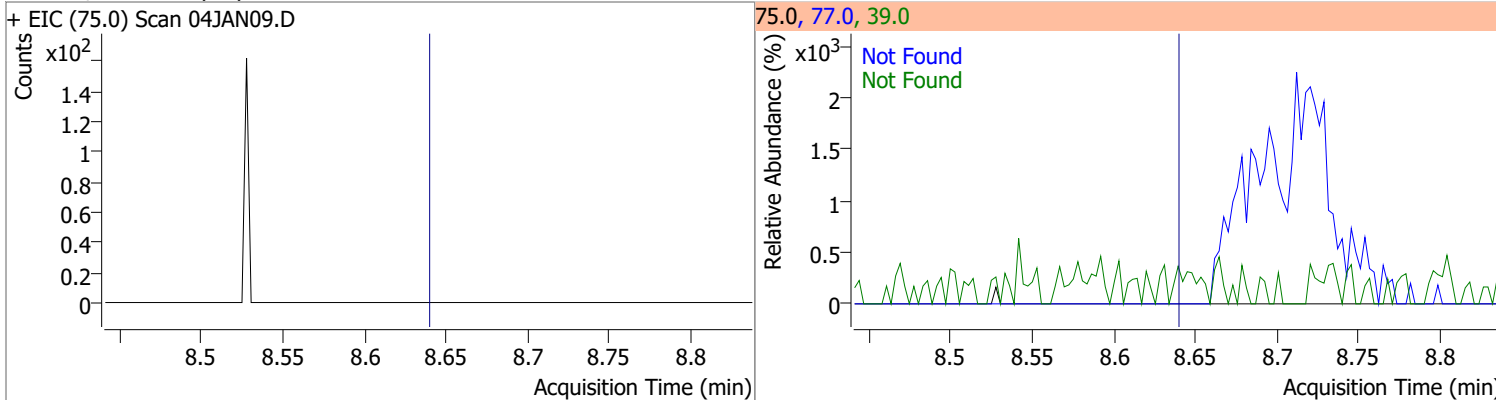









| Compound              | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------------|-------|--------|------|-----------|------|-----------|
| 1,1,2-Trichloroethane | N.D.  | 8.82   | 97.0 | 114.6     | 85.0 | 67.6      |

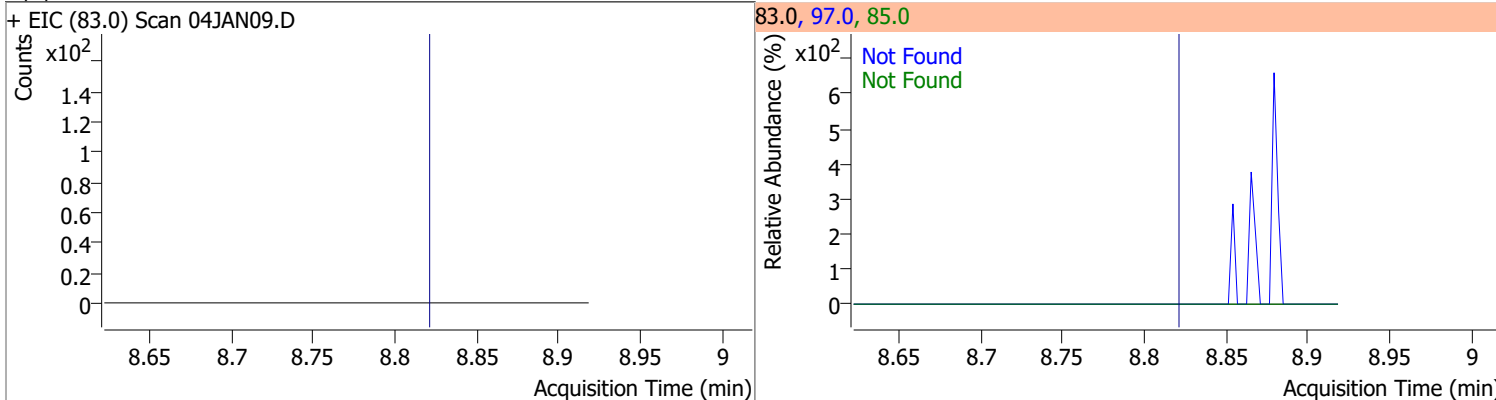




# Quantitation Results Report (QT Reviewed)
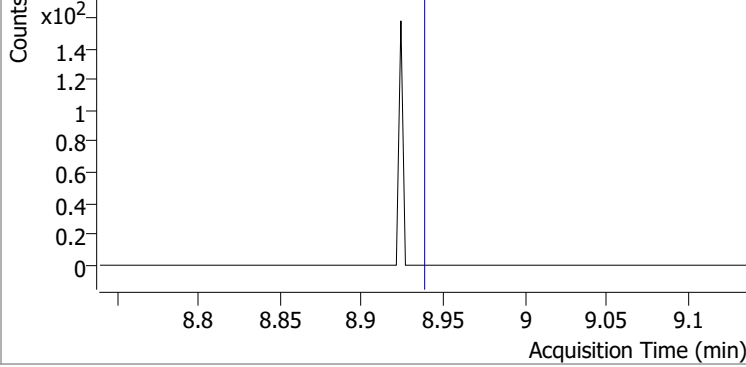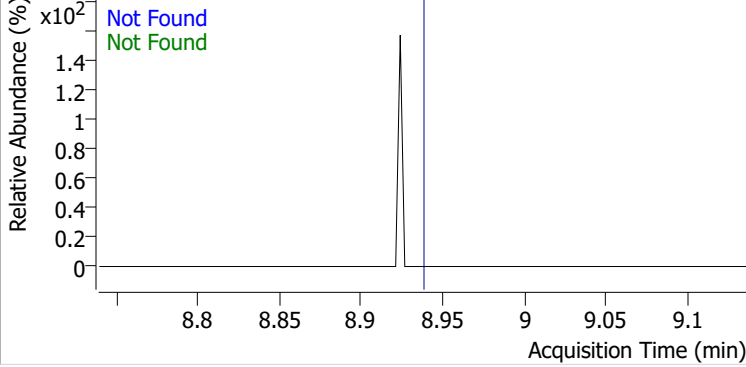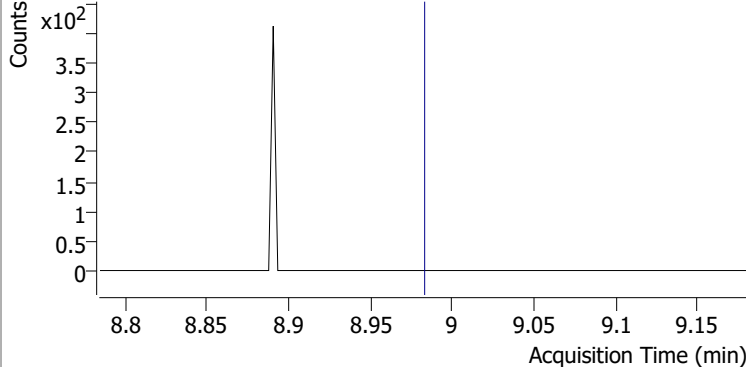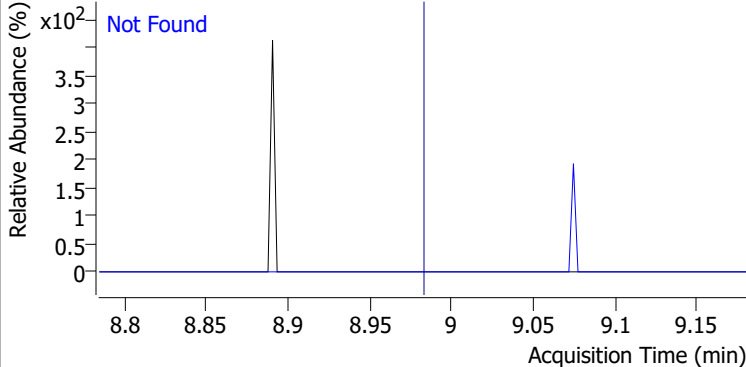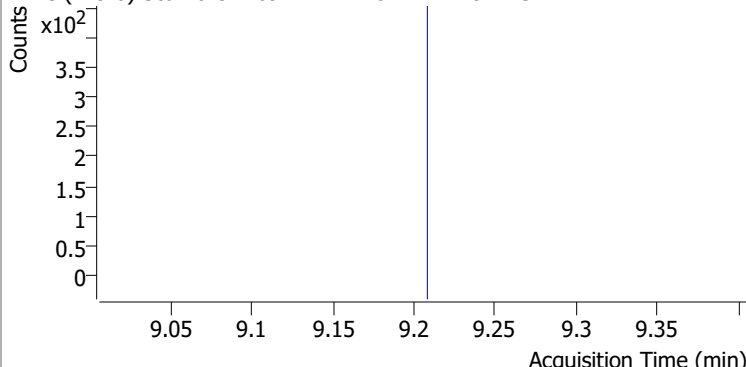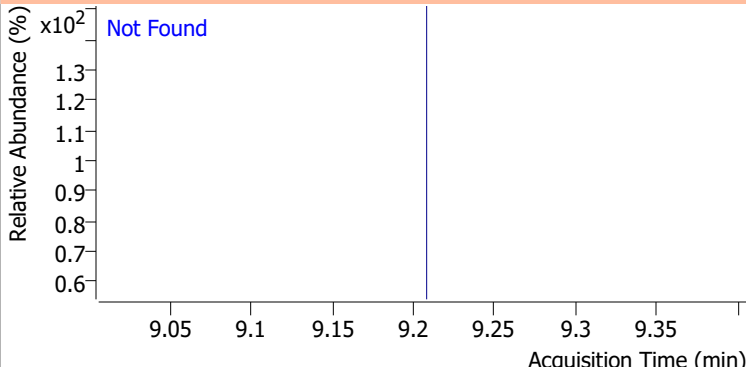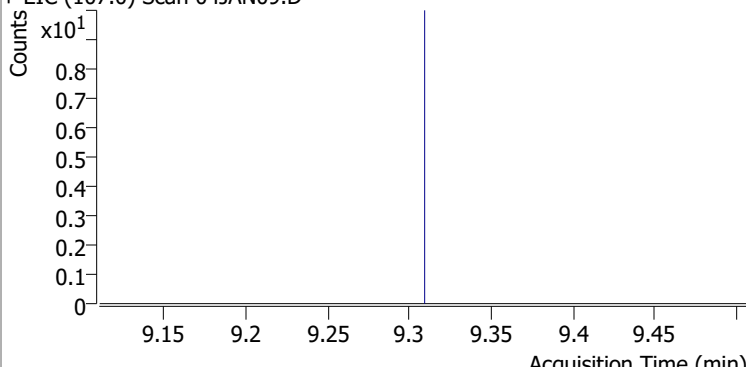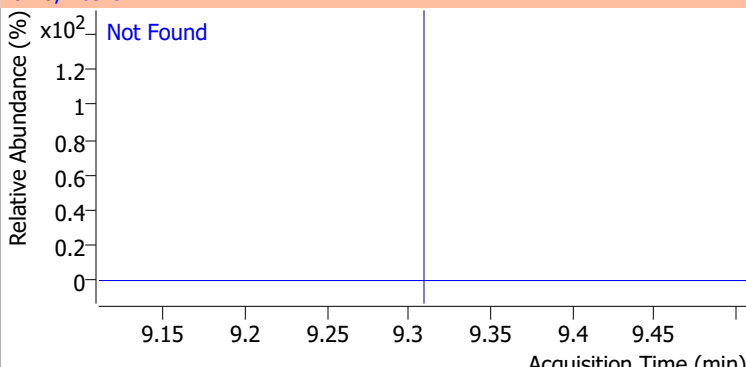
| Compound                                                                           | Conc. | Exp RT | QIon                                                                                 | Exp Ratio | QIon  | Exp Ratio |
|------------------------------------------------------------------------------------|-------|--------|--------------------------------------------------------------------------------------|-----------|-------|-----------|
| Tetrachloroethene                                                                  | N.D.  | 8.94   | 165.8                                                                                | 128.6     | 129.0 | 91.5      |
| + EIC (163.8) Scan 04JAN09.D                                                       |       |        | 163.8, 129.0, 165.8                                                                  |           |       |           |
|    |       |        |    |           |       |           |
| 1,3-Dichloropropane                                                                | N.D.  | 8.98   | 78.0                                                                                 | 32.9      |       |           |
| + EIC (76.0) Scan 04JAN09.D                                                        |       |        | 76.0, 78.0                                                                           |           |       |           |
|   |       |        |   |           |       |           |
| Chlorodibromomethane                                                               | N.D.  | 9.21   | 127.0                                                                                | 78.0      |       |           |
| + EIC (129.0) Scan 04JAN09.D ***NO DATA POINTS***                                  |       |        | 129.0, 127.0                                                                         |           |       |           |
|  |       |        |  |           |       |           |
| 1,2-Dibromoethane                                                                  | N.D.  | 9.31   | 109.0                                                                                | 94.5      |       |           |
| + EIC (107.0) Scan 04JAN09.D                                                       |       |        | 107.0, 109.0                                                                         |           |       |           |
|  |       |        |  |           |       |           |


# Quantitation Results Report (QT Reviewed)
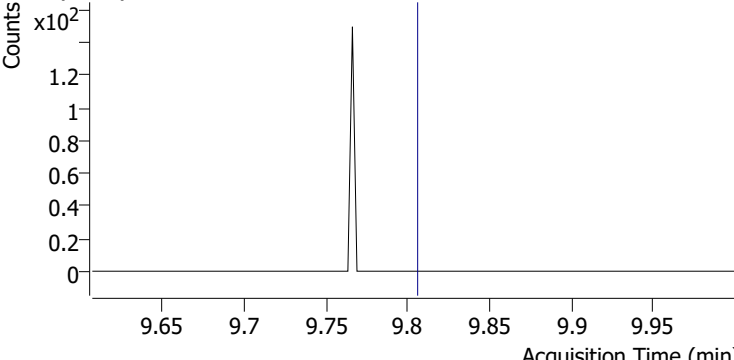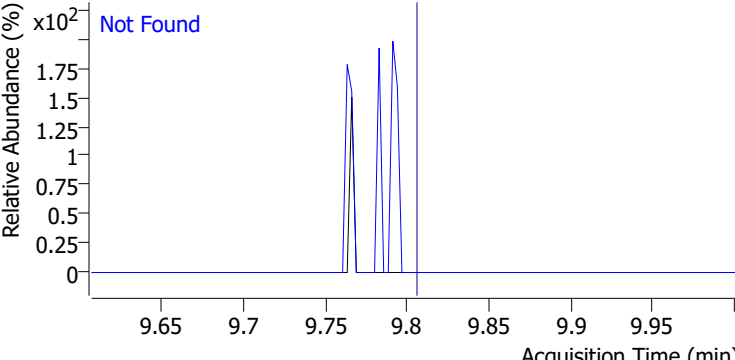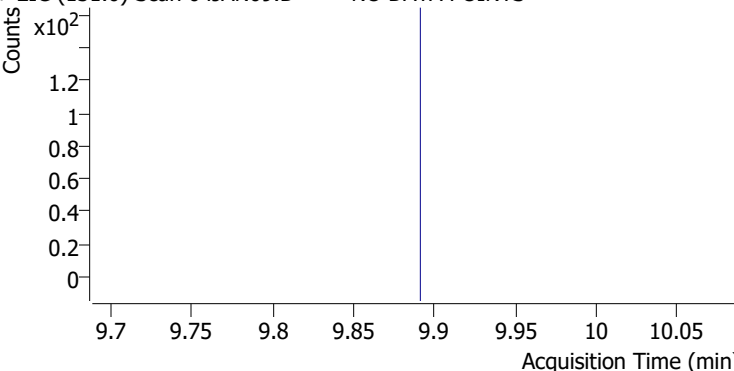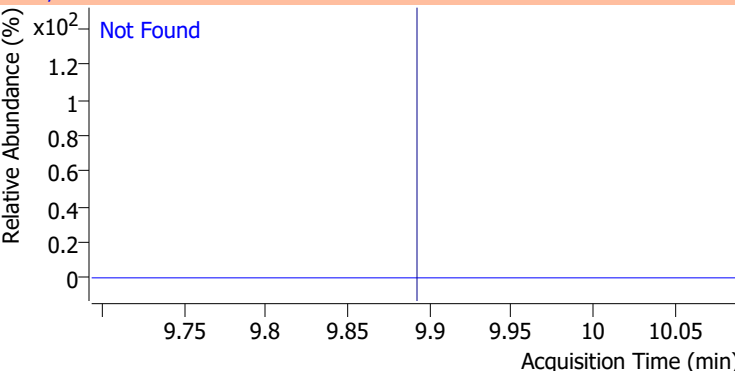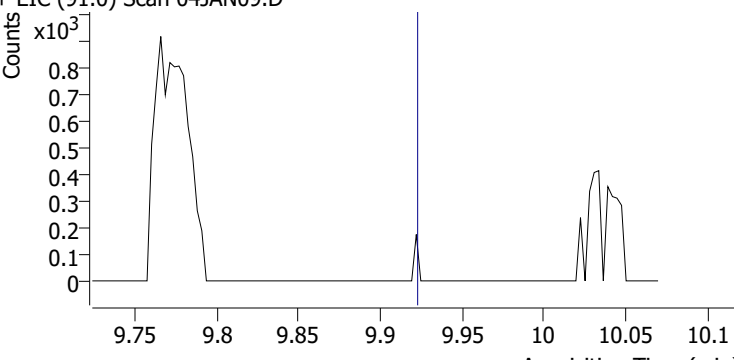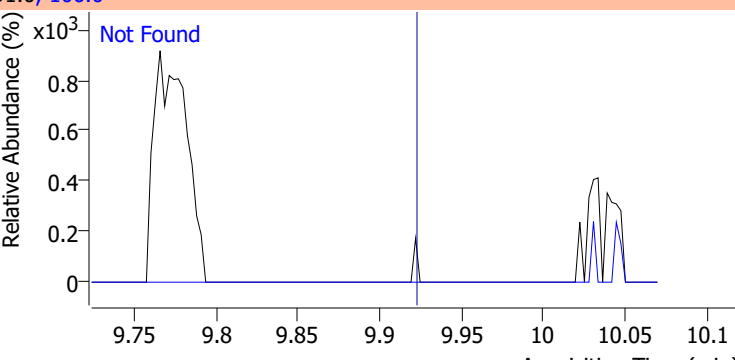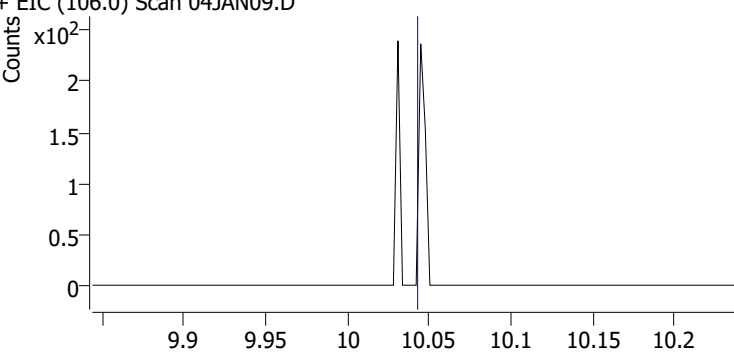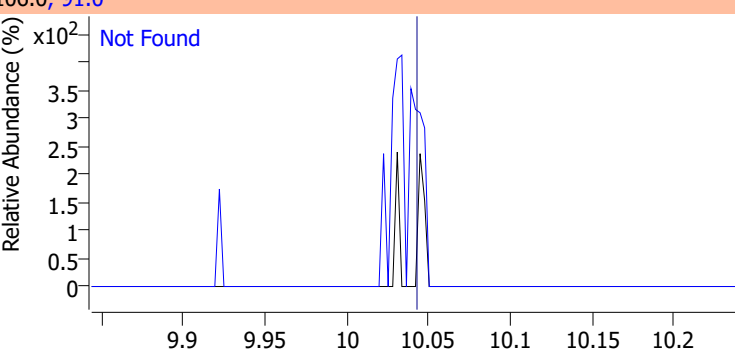
| Compound                                                                           | Conc. | Exp RT | QIon                                                                                 | Exp Ratio |
|------------------------------------------------------------------------------------|-------|--------|--------------------------------------------------------------------------------------|-----------|
| Chlorobenzene                                                                      | N.D.  | 9.80   | 114.0                                                                                | 32.1      |
| + EIC (112.0) Scan 04JAN09.D                                                       |       |        | 112.0, 114.0                                                                         |           |
|    |       |        |    |           |
| 1,1,1,2-Tetrachloroethane                                                          | N.D.  | 9.89   | 133.0                                                                                | 98.6      |
| + EIC (131.0) Scan 04JAN09.D ***NO DATA POINTS***                                  |       |        | 131.0, 133.0                                                                         |           |
|    |       |        |    |           |
| Ethylbenzene                                                                       | N.D.  | 9.92   | 106.0                                                                                | 31.1      |
| + EIC (91.0) Scan 04JAN09.D                                                        |       |        | 91.0, 106.0                                                                          |           |
|  |       |        |  |           |
| m+p-Xylenes                                                                        | N.D.  | 10.04  | 91.0                                                                                 | 201.4     |
| + EIC (106.0) Scan 04JAN09.D                                                       |       |        | 106.0, 91.0                                                                          |           |
|  |       |        |  |           |

# Quantitation Results Report (QT Reviewed)

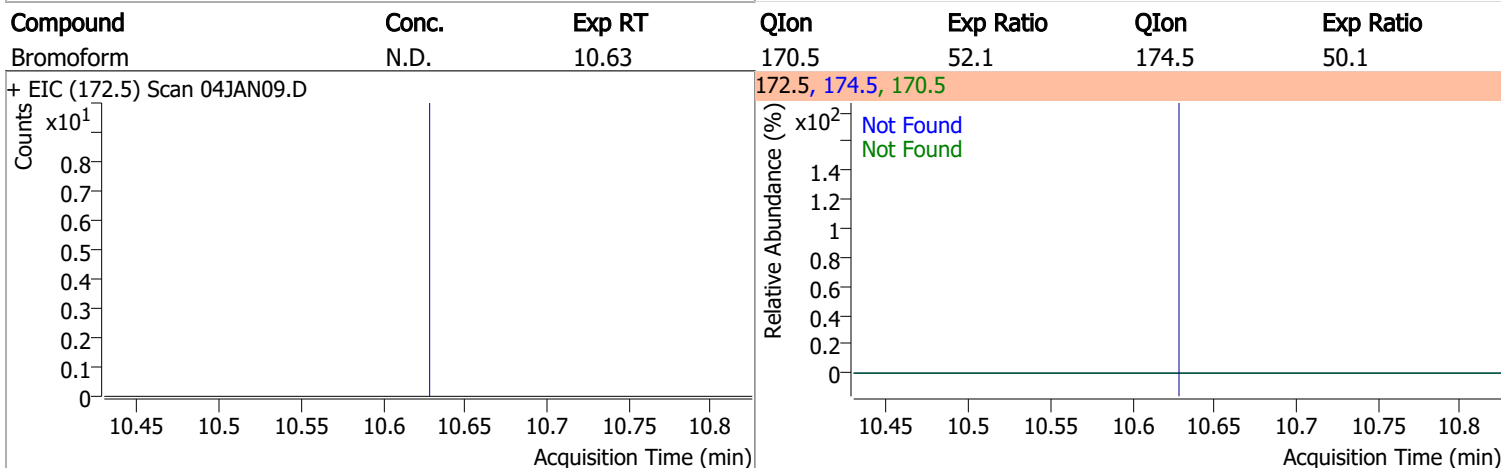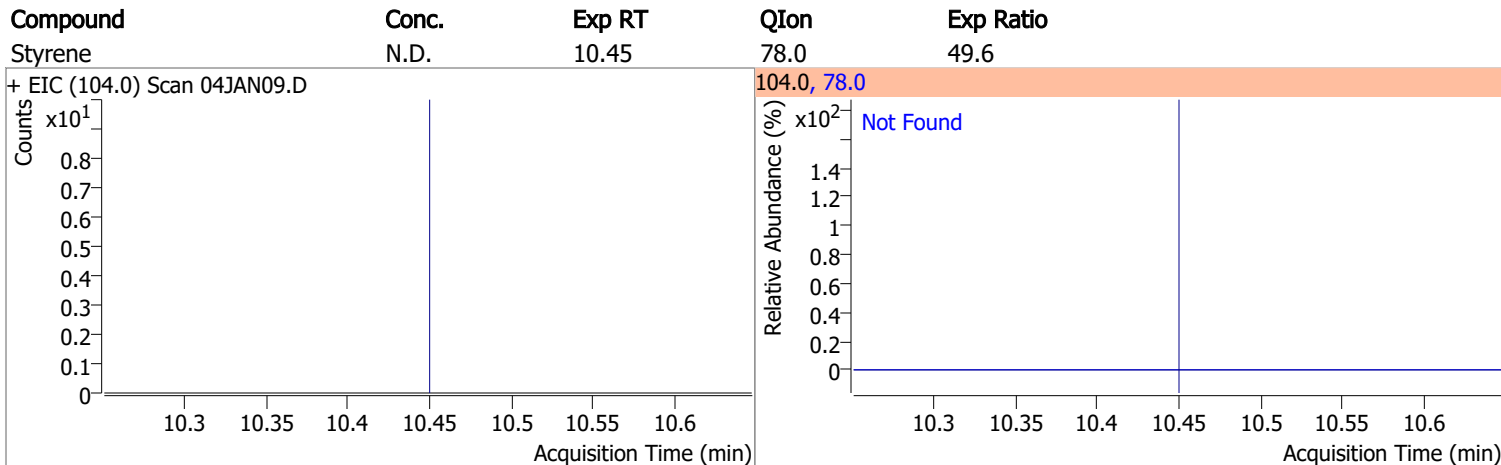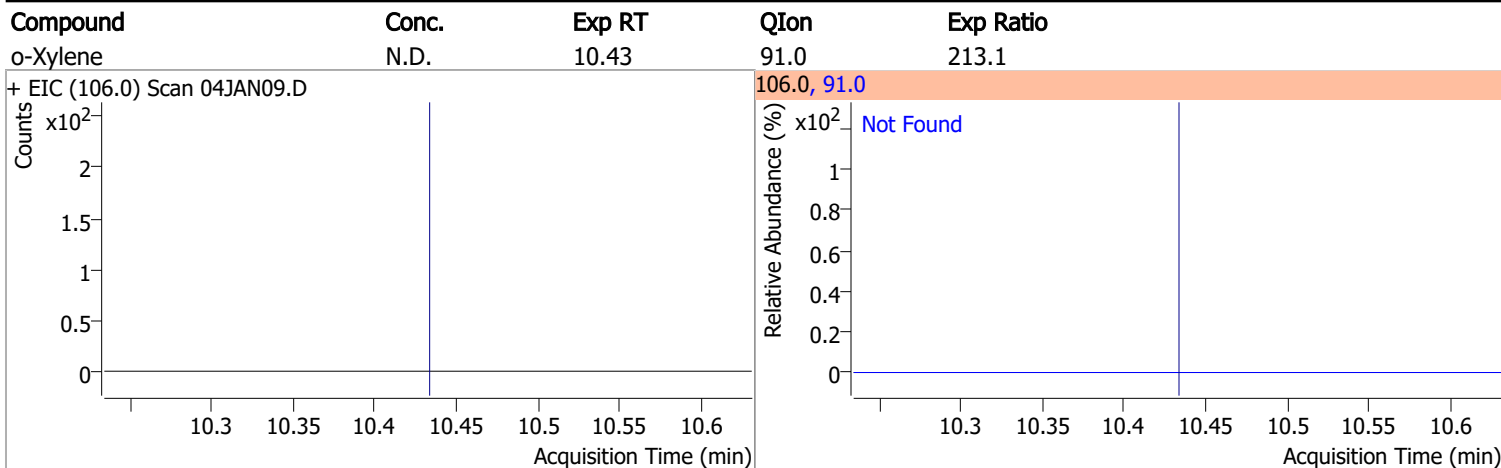









| Compound             | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 267.2815 | 10.95 | 0.00     | 226743 | 174.0 | 95.5   | 61.7  | 121.7 |
|                      |          |       |          |        | 176.0 | 91.1   | 60.6  | 120.6 |

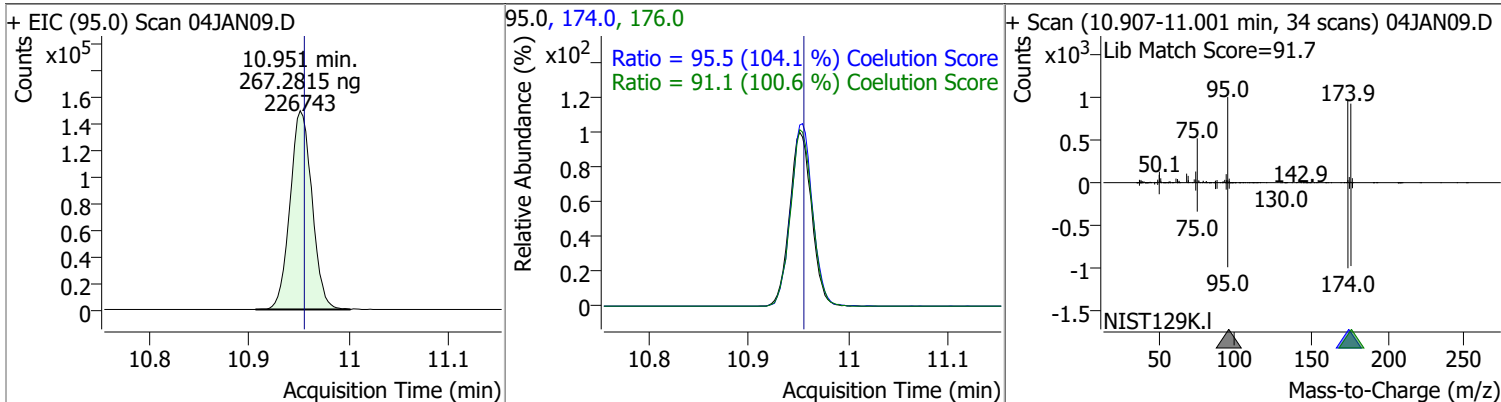

# Quantitation Results Report (QT Reviewed)

| Compound                                          | Conc. | Exp RT | QIon               | Exp Ratio | QIon  | Exp Ratio |
|---------------------------------------------------|-------|--------|--------------------|-----------|-------|-----------|
| Bromobenzene                                      | N.D.  | 11.09  | 77.0               | 145.7     | 158.0 | 96.5      |
| + EIC (156.0) Scan 04JAN09.D ***NO DATA POINTS*** |       |        | 156.0, 77.0, 158.0 |           |       |           |
|                                                   |       |        |                    |           |       |           |
| 1,1,2,2-Tetrachloroethane                         | N.D.  | 11.12  | 85.0               | 66.2      |       |           |
| + EIC (83.0) Scan 04JAN09.D                       |       |        | 83.0, 85.0         |           |       |           |
|                                                   |       |        |                    |           |       |           |
| 1,2,3-Trichloropropane                            | N.D.  | 11.15  | 112.0              | 63.5      |       |           |
| + EIC (110.0) Scan 04JAN09.D                      |       |        | 110.0, 112.0       |           |       |           |
|                                                   |       |        |                    |           |       |           |
| 2-Chlorotoluene                                   | N.D.  | 11.29  | 91.0               | 282.3     |       |           |
| + EIC (126.0) Scan 04JAN09.D ***NO DATA POINTS*** |       |        | 126.0, 91.0        |           |       |           |
|                                                   |       |        |                    |           |       |           |


# Quantitation Results Report (QT Reviewed)
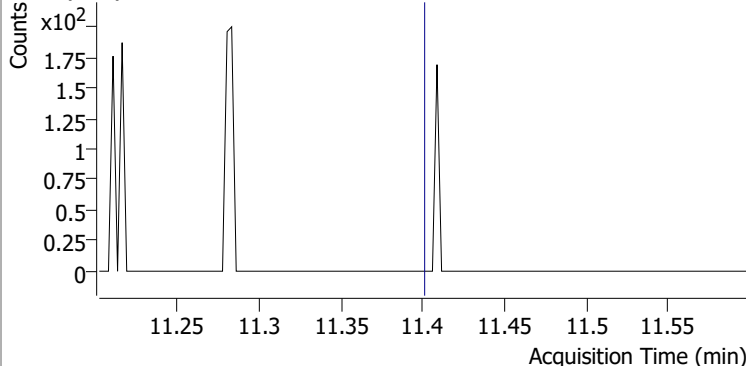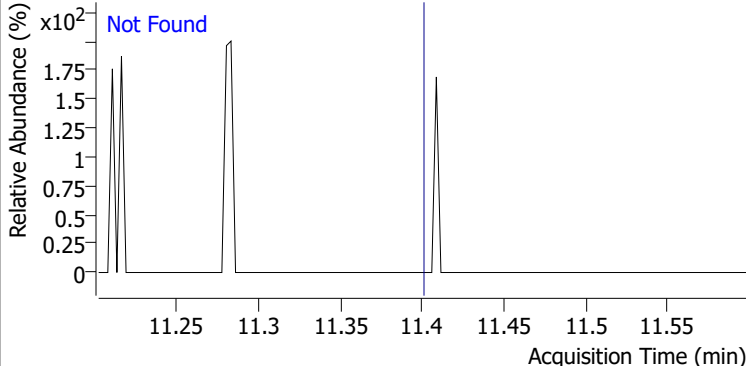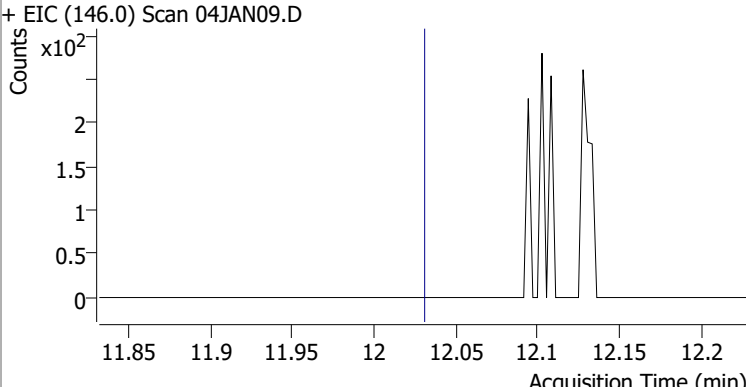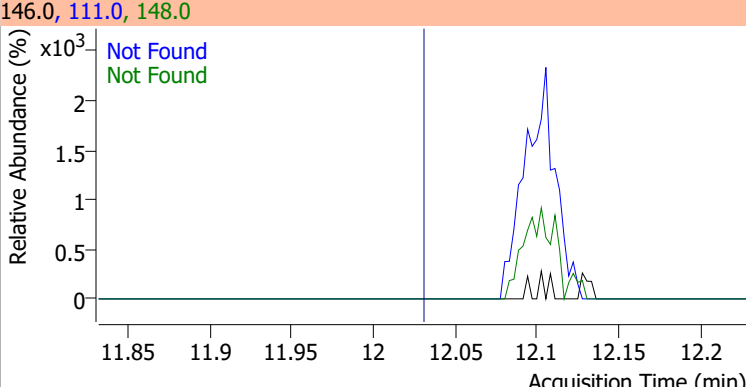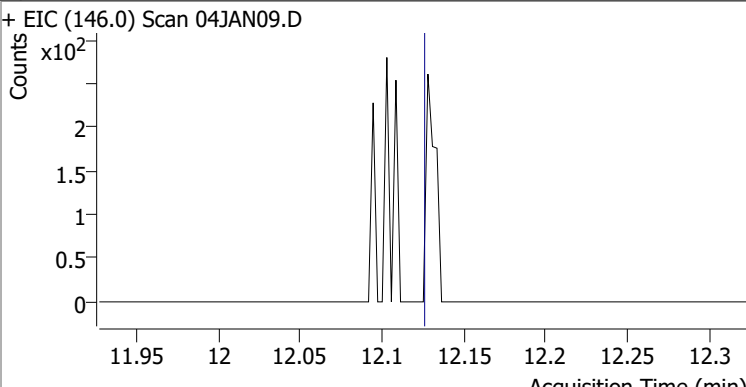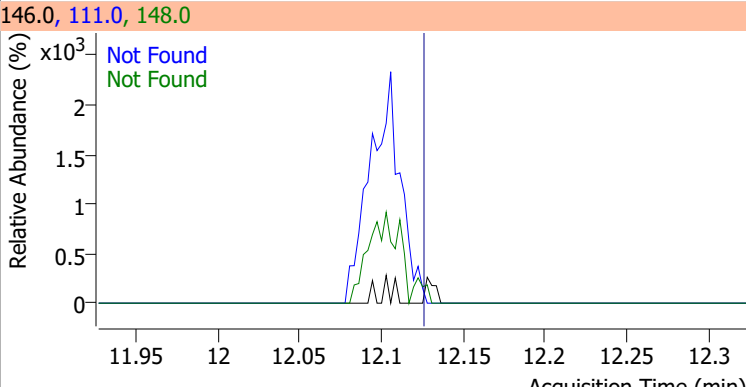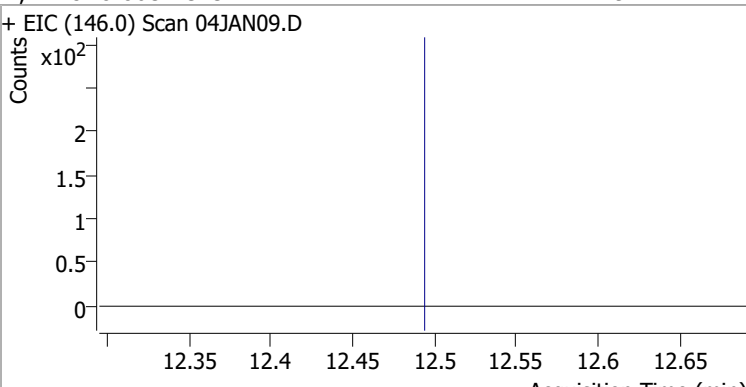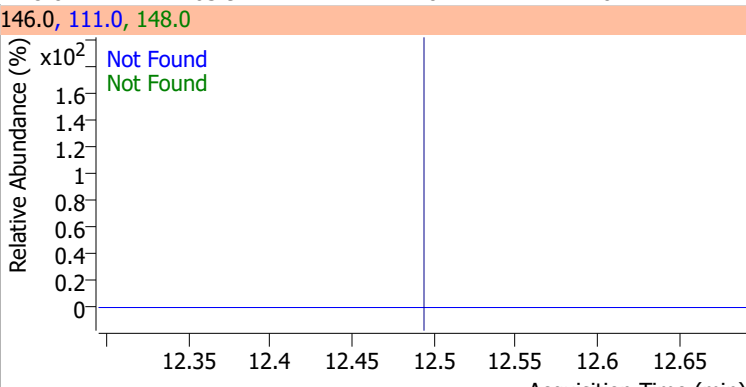
| Compound                                                                           | Conc. | Exp RT | QIon                                                                                 | Exp Ratio |      |           |
|------------------------------------------------------------------------------------|-------|--------|--------------------------------------------------------------------------------------|-----------|------|-----------|
| 4-Chlorotoluene                                                                    | N.D.  | 11.40  | 126.0                                                                                | 31.7      |      |           |
| + EIC (91.0) Scan 04JAN09.D                                                        |       |        | 91.0, 126.0                                                                          |           |      |           |
|    |       |        |    |           |      |           |
| 1,3-Dichlorobenzene                                                                | N.D.  | 12.03  | 148.0                                                                                | 63.6      | QIon | Exp Ratio |
| + EIC (146.0) Scan 04JAN09.D                                                       |       |        | 146.0, 111.0, 148.0                                                                  |           |      |           |
|   |       |        |   |           |      |           |
| 1,4-Dichlorobenzene                                                                | N.D.  | 12.13  | 148.0                                                                                | 63.1      | QIon | Exp Ratio |
| + EIC (146.0) Scan 04JAN09.D                                                       |       |        | 146.0, 111.0, 148.0                                                                  |           |      |           |
|  |       |        |  |           |      |           |
| 1,2-Dichlorobenzene                                                                | N.D.  | 12.49  | 148.0                                                                                | 63.9      | QIon | Exp Ratio |
| + EIC (146.0) Scan 04JAN09.D                                                       |       |        | 146.0, 111.0, 148.0                                                                  |           |      |           |
|  |       |        |  |           |      |           |



# Quantitation Results Report (QT Reviewed)

|                |                                     |                   |                       |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File      | 04JAN10.D                           | Operator          | MSC                   |
| Acq. Method    | 5975CACQF.M                         | Acq. Date-Time    | 1/4/2022 3:33:04 PM   |
| Sample Name    | ICAL010422_1                        | Instrument        | VOA5975C              |
| Vial           | 10                                  | Multiplier        | 1.00                  |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m  | Comment           |                       |
| Tune File      | BFB_Atune3.u                        | Tune Date         | 10/11/2021 4:02:00 PM |
| Batch Name     | VG010422_8260B.batch.bin            | Last Calib Update | 1/9/2022 8:59:52 PM   |
| Ref Library    | \\MASSHUNTER\Org\Library\NIST129K.l |                   |                       |

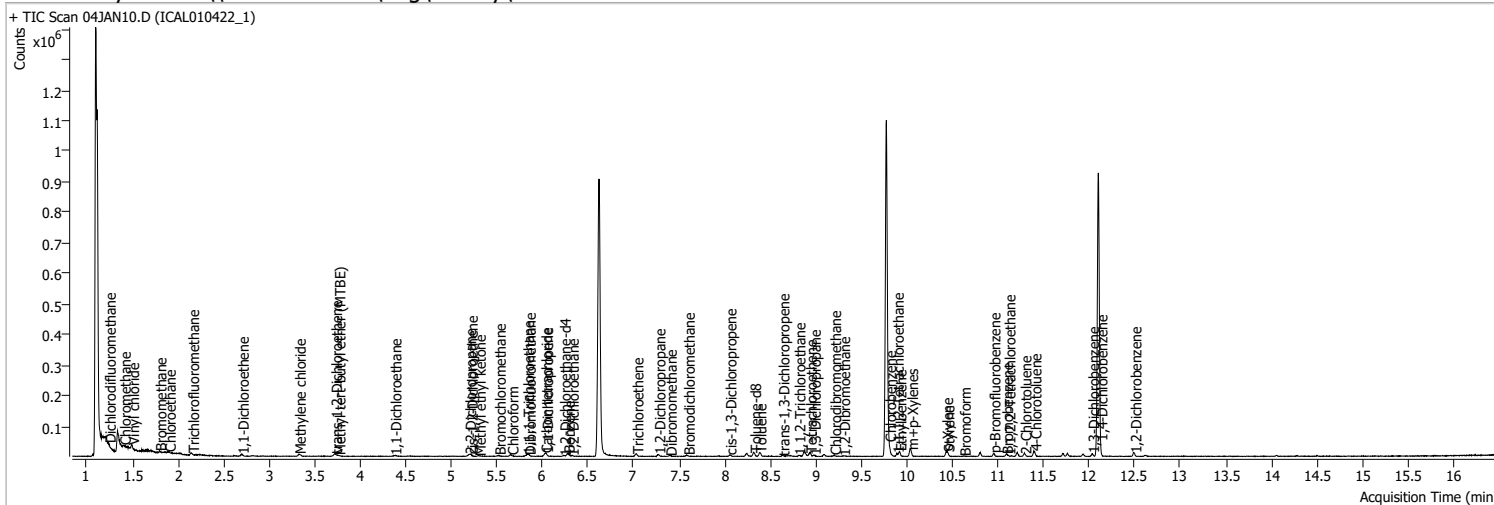

| Compound                           | RT                   | QIon  | Resp.  | Conc.            | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|------------------|-------|----------|
| <b>Internal Standards</b>          |                      |       |        |                  |       |          |
| M Fluorobenzene                    | 6.621                | 96.0  | 770895 | 250.0000         | ng    | -0.003   |
| M Chlorobenzene-d5                 | 9.772                | 82.0  | 296081 | 250.0000         | ng    | 0.000    |
| M 1,4-Dichlorobenzene-d4           | 12.100               | 152.0 | 227879 | 250.0000         | ng    | 0.000    |
| <b>System Monitoring Compounds</b> |                      |       |        |                  |       |          |
| S Dibromofluoromethane             | 5.851                | 113.0 | 2508   | 3.4533           | ng    | m 0.006  |
| Spiked Amount: 250.000             | Range: 80.0 - 119.0% |       |        | Recovery = 1.38% |       | *        |
| S 1,2-Dichloroethane-d4            | 6.233                | 67.0  | 923    | 2.9438           | ng    | m 0.000  |
| Spiked Amount: 250.000             | Range: 81.0 - 118.0% |       |        | Recovery = 1.18% |       | *        |
| S Toluene-d8                       | 8.322                | 98.0  | 7777   | 2.7257           | ng    | 0.003    |
| Spiked Amount: 250.000             | Range: 89.0 - 112.0% |       |        | Recovery = 1.09% |       | *        |
| S p-Bromofluorobenzene             | 10.951               | 95.0  | 2719   | 3.2569           | ng    | -0.003   |
| Spiked Amount: 250.000             | Range: 85.0 - 114.0% |       |        | Recovery = 1.30% |       | *        |
| <b>Target Compounds</b>            |                      |       |        |                  |       |          |
| T Dichlorodifluoromethane          | 1.241                | 85.0  | 4353   | 4.3090           | ng    | 99       |
| T Chloromethane                    | 1.406                | 50.0  | 7435   | 6.0637           | ng    | 83       |
| T Vinyl chloride                   | 1.495                | 62.0  | 4274   | 3.8739           | ng    | 94       |
| T Bromomethane                     | 1.796                | 96.0  | 1902   | 3.8547           | ng    | m 88     |
| T Chloroethane                     | 1.899                | 64.0  | 2178   | 3.9871           | ng    | m 86     |
| T Trichlorofluoromethane           | 2.153                | 101.0 | 5030   | 3.6731           | ng    | 91       |
| T 1,1-Dichloroethene               | 2.700                | 96.0  | 2084   | 2.6839           | ng    | m 95     |
| T Methylene chloride               | 3.324                | 49.0  | 4095   | 3.5774           | ng    | 88       |
| T trans-1,2-Dichloroethene         | 3.723                | 96.0  | 2146   | 2.7090           | ng    | m 100    |
| T Methyl tert-butyl ether (MTBE)   | 3.759                | 73.0  | 2717   | 2.6532           | ng    | m 90     |
| T 1,1-Dichloroethane               | 4.376                | 63.0  | 3892   | 2.6393           | ng    | 91       |
| T 2,2-Dichloropropane              | 5.196                | 77.0  | 2930   | 2.6520           | ng    | m 88     |
| T cis-1,2-Dichloroethene           | 5.212                | 96.0  | 2376   | 2.9581           | ng    | m 95     |
| T Methyl ethyl ketone              | 5.302                | 43.0  | 3035   | 27.8967          | ng    | 85       |
| T Bromochloromethane               | 5.522                | 128.0 | 807    | 2.4260           | ng    | m 82     |
| T Chloroform                       | 5.659                | 83.0  | 4248   | 2.8946           | ng    | 97       |


# Quantitation Results Report (QT Reviewed)

| Compound                    | RT     | QIon  | Resp. | Conc.  | Units | Dev(Min) |
|-----------------------------|--------|-------|-------|--------|-------|----------|
| T 1,1,1-Trichloroethane     | 5.831  | 97.0  | 3510  | 2.5521 | ng    | 99       |
| T Carbon tetrachloride      | 6.029  | 117.0 | 4342  | 3.2043 | ng    | 77       |
| T 1,1-Dichloropropene       | 6.041  | 75.0  | 2830  | 2.4201 | ng    | 91       |
| T Benzene                   | 6.278  | 78.0  | 8408  | 2.7393 | ng    | 98       |
| T 1,2-Dichloroethane        | 6.322  | 62.0  | 2415  | 2.9090 | ng m  | 96       |
| T Trichloroethene           | 7.033  | 95.0  | 2372  | 2.6564 | ng m  | 93       |
| T 1,2-Dichloropropane       | 7.273  | 63.0  | 2148  | 2.7347 | ng    | 93       |
| T Dibromomethane            | 7.396  | 93.0  | 902   | 2.7162 | ng m  | 88       |
| T Bromodichloromethane      | 7.597  | 83.0  | 2536  | 2.7684 | ng    | 98       |
| T cis-1,3-Dichloropropene   | 8.054  | 75.0  | 2583  | 2.4939 | ng    | 94       |
| T Toluene                   | 8.380  | 92.0  | 5039  | 2.6145 | ng    | 93       |
| T trans-1,3-Dichloropropene | 8.634  | 75.0  | 1470  | 1.9942 | ng m  | 83       |
| T 1,1,2-Trichloroethane     | 8.810  | 83.0  | 960   | 2.5012 | ng m  | 89       |
| T Tetrachloroethene         | 8.932  | 163.8 | 2105  | 2.6772 | ng m  | 95       |
| T 1,3-Dichloropropane       | 8.977  | 76.0  | 2257  | 2.9881 | ng    | 77       |
| T Chlorodibromomethane      | 9.203  | 129.0 | 1468  | 2.4461 | ng m  | 100      |
| T 1,2-Dibromoethane         | 9.300  | 107.0 | 1299  | 3.0943 | ng m  | 85       |
| T Chlorobenzene             | 9.805  | 112.0 | 5771  | 2.7350 | ng    | 100      |
| T 1,1,1,2-Tetrachloroethane | 9.889  | 131.0 | 1893  | 2.5659 | ng m  | 98       |
| T Ethylbenzene              | 9.920  | 91.0  | 9283  | 2.5367 | ng    | 93       |
| T m+p-Xylenes               | 10.045 | 106.0 | 7212  | 5.0712 | ng    | 88       |
| T o-Xylene                  | 10.430 | 106.0 | 3330  | 2.6303 | ng #  | 80       |
| T Styrene                   | 10.444 | 104.0 | 4408  | 2.1625 | ng    | 98       |
| T Bromoform                 | 10.625 | 172.5 | 708   | 2.4287 | ng m  | 87       |
| T Bromobenzene              | 11.088 | 156.0 | 2024  | 2.7439 | ng m  | 94       |
| T 1,1,2,2-Tetrachloroethane | 11.113 | 83.0  | 1142  | 2.6916 | ng m  | 92       |
| T 1,2,3-Trichloropropane    | 0.000  |       | 0     | N.D.   |       |          |
| T 2-Chlorotoluene           | 11.292 | 126.0 | 1844  | 2.5124 | ng m  | 97       |
| T 4-Chlorotoluene           | 11.400 | 91.0  | 5419  | 2.2650 | ng    | 96       |
| T 1,3-Dichlorobenzene       | 12.033 | 146.0 | 3541  | 2.6327 | ng    | 99       |
| T 1,4-Dichlorobenzene       | 12.125 | 146.0 | 3787  | 2.7613 | ng    | 90       |
| T 1,2-Dichlorobenzene       | 12.499 | 146.0 | 3104  | 2.7307 | ng    | 96       |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (\*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

# Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|-------|----|----------|-------|------|--------|-------|-------|
|----------|-------|----|----------|-------|------|--------|-------|-------|

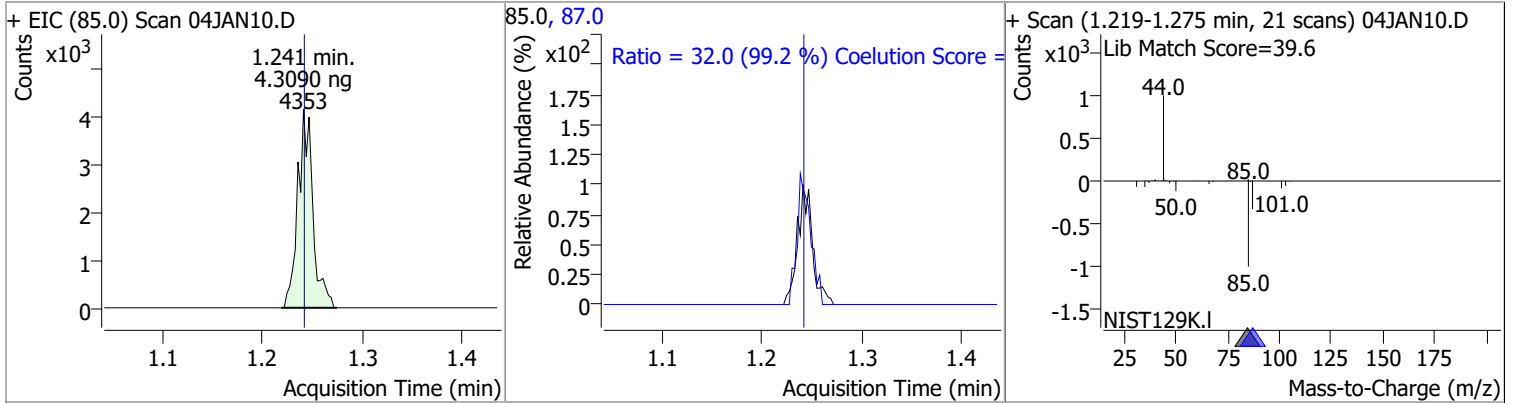


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|-------|----|----------|-------|------|--------|-------|-------|
|----------|-------|----|----------|-------|------|--------|-------|-------|

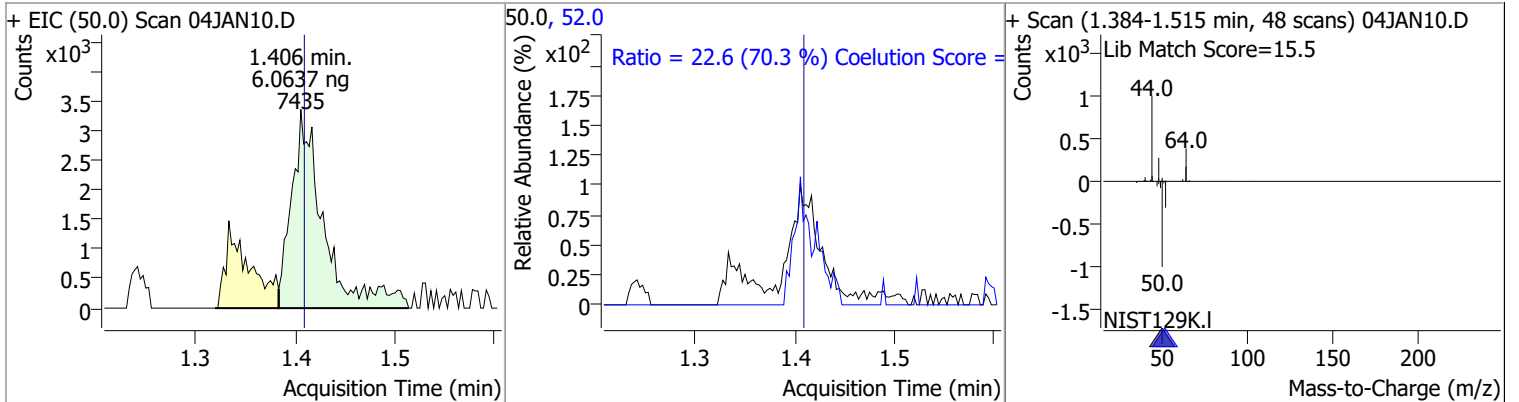

| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|-------|----|----------|-------|------|--------|-------|-------|
|----------|-------|----|----------|-------|------|--------|-------|-------|

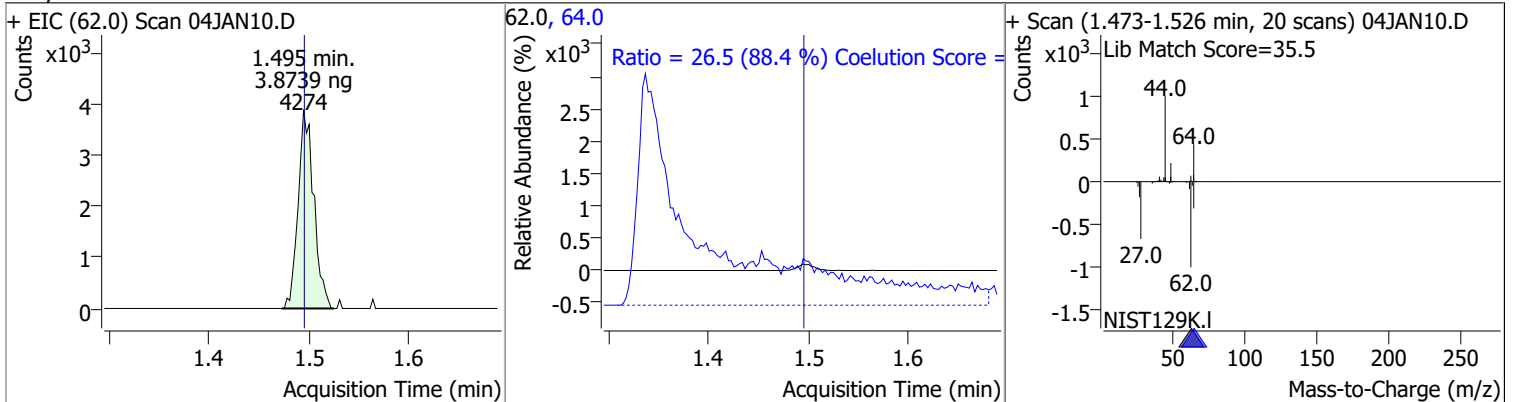


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|-------|----|----------|-------|------|--------|-------|-------|
|----------|-------|----|----------|-------|------|--------|-------|-------|

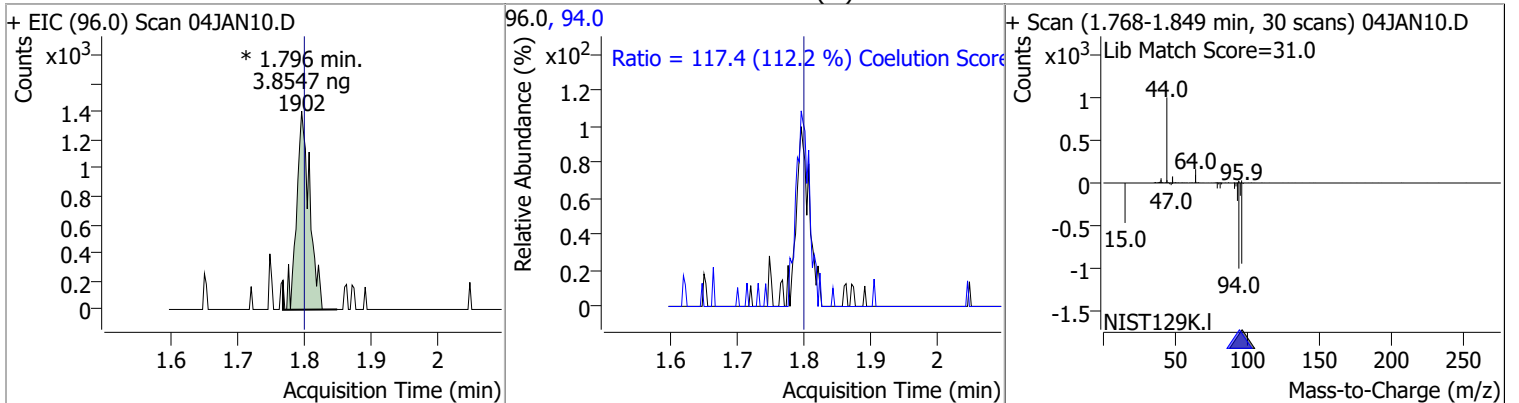


# Quantitation Results Report (QT Reviewed)


| Compound     | Conc.  | RT   | Dev(Min) | Resp.    | QIon | QRatio | Lower | Upper |
|--------------|--------|------|----------|----------|------|--------|-------|-------|
| Chloroethane | 3.9871 | 1.90 | 0.01     | 2178 (m) | 66.0 | 37.9   | 0.1   | 60.1  |




|                        |        |      |      |      |       |      |      |      |
|------------------------|--------|------|------|------|-------|------|------|------|
| Trichlorofluoromethane | 3.6731 | 2.15 | 0.01 | 5030 | 103.0 | 57.3 | 34.2 | 94.2 |
|------------------------|--------|------|------|------|-------|------|------|------|



|                    |        |      |      |          |      |       |       |       |
|--------------------|--------|------|------|----------|------|-------|-------|-------|
| 1,1-Dichloroethene | 2.6839 | 2.70 | 0.00 | 2084 (m) | 61.0 | 188.1 | 150.3 | 210.3 |
|                    |        |      |      |          | 63.0 | 55.5  | 26.7  | 86.7  |




|                    |        |      |       |      |      |      |      |      |
|--------------------|--------|------|-------|------|------|------|------|------|
| Methylene chloride | 3.5774 | 3.32 | -0.01 | 4095 | 84.0 | 82.8 | 36.9 | 96.9 |
|                    |        |      |       |      | 86.0 | 44.4 | 14.3 | 74.3 |




# Quantitation Results Report (QT Reviewed)


| Compound                 | Conc.  | RT   | Dev(Min) | Resp.    | QIon | QRatio | Lower | Upper |
|--------------------------|--------|------|----------|----------|------|--------|-------|-------|
| trans-1,2-Dichloroethene | 2.7090 | 3.72 | 0.01     | 2146 (m) | 61.0 | 153.6  | 123.9 | 183.9 |
|                          |        |      |          |          | 98.0 | 66.5   | 35.7  | 95.7  |



| Compound                       | Conc.  | RT   | Dev(Min) | Resp.    | QIon | QRatio | Lower | Upper |
|--------------------------------|--------|------|----------|----------|------|--------|-------|-------|
| Methyl tert-butyl ether (MTBE) | 2.6532 | 3.76 | 0.01     | 2717 (m) | 57.0 | 19.6   | 0.0   | 54.6  |
|                                |        |      |          |          |      |        |       |       |




| Compound           | Conc.  | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|--------|------|----------|-------|------|--------|-------|-------|
| 1,1-Dichloroethane | 2.6393 | 4.38 | 0.00     | 3892  | 65.0 | 34.6   | 2.1   | 62.1  |
|                    |        |      |          |       | 83.0 | 5.8    | 0.0   | 43.7  |




# Quantitation Results Report (QT Reviewed)


| Compound            | Conc.  | RT   | Dev(Min) | Resp.    | QIon | QRatio | Lower | Upper |
|---------------------|--------|------|----------|----------|------|--------|-------|-------|
| 2,2-Dichloropropane | 2.6520 | 5.20 | 0.00     | 2930 (m) | 41.0 | 76.7   | 36.5  | 96.5  |
|                     |        |      |          |          | 97.0 | 27.8   | 0.0   | 53.2  |

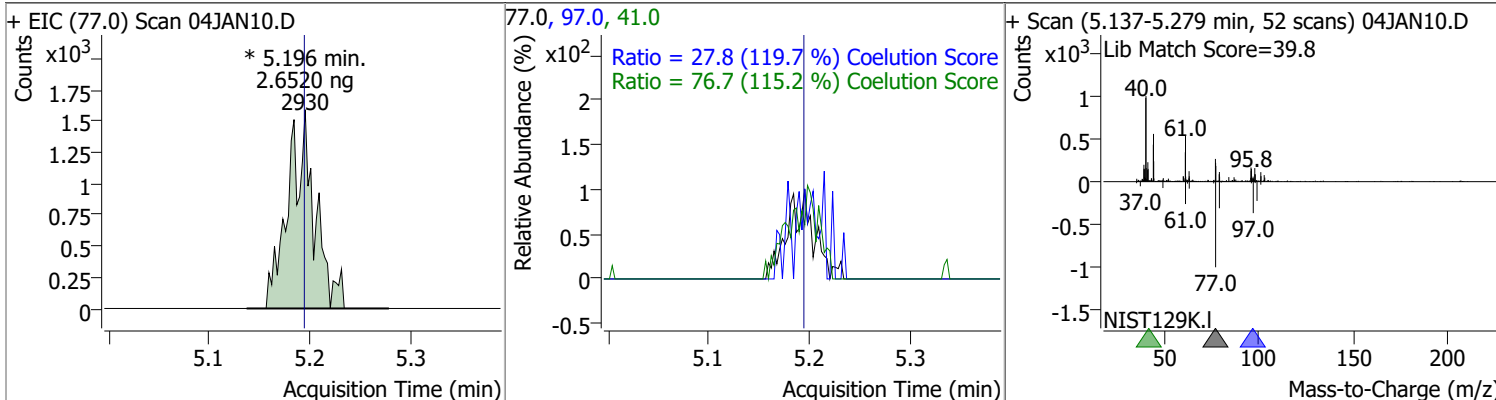


| Compound               | Conc.  | RT   | Dev(Min) | Resp.    | QIon | QRatio | Lower | Upper |
|------------------------|--------|------|----------|----------|------|--------|-------|-------|
| cis-1,2-Dichloroethene | 2.9581 | 5.21 | 0.00     | 2376 (m) | 61.0 | 174.2  | 137.2 | 197.2 |
|                        |        |      |          |          | 98.0 | 64.2   | 37.3  | 97.3  |

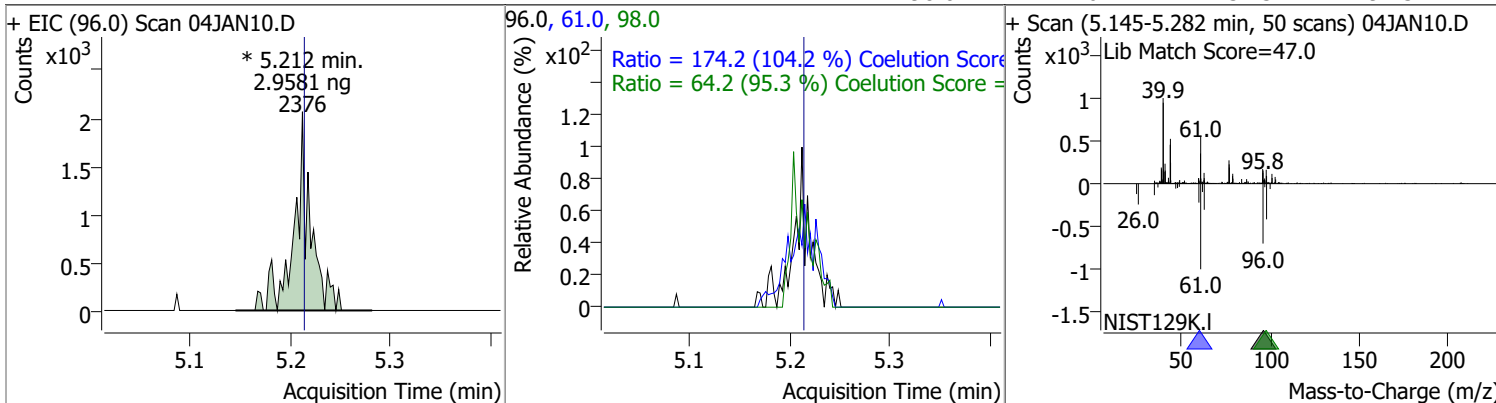

| Compound            | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|---------|------|----------|-------|------|--------|-------|-------|
| Methyl ethyl ketone | 27.8967 | 5.30 | 0.02     | 3035  | 72.0 | 14.3   | 0.0   | 51.3  |

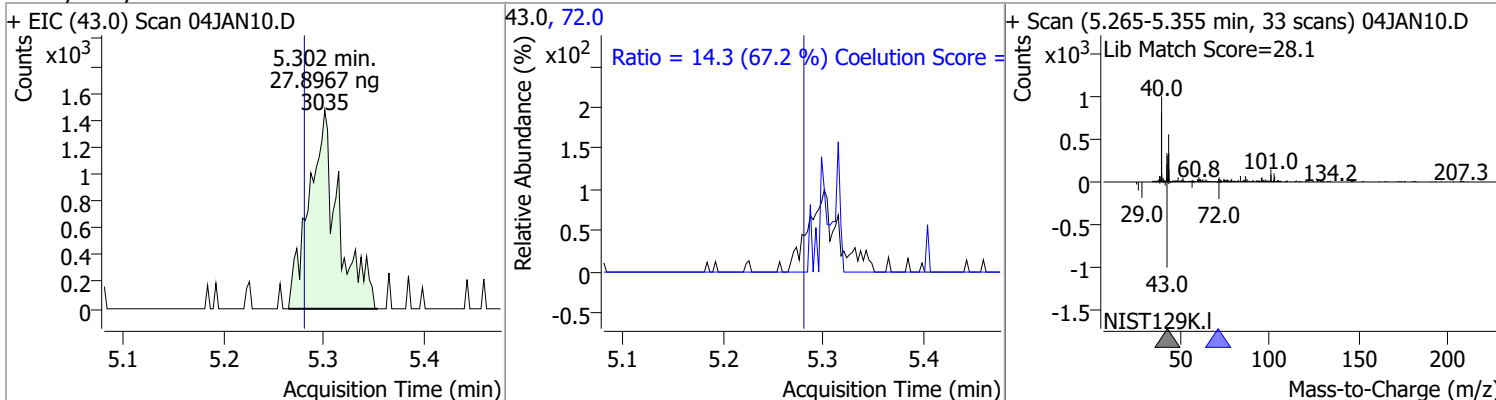


| Compound           | Conc.  | RT   | Dev(Min) | Resp.   | QIon | QRatio | Lower | Upper |
|--------------------|--------|------|----------|---------|------|--------|-------|-------|
| Bromochloromethane | 2.4260 | 5.52 | 0.00     | 807 (m) | 49.0 | 208.8  | 152.9 | 212.9 |

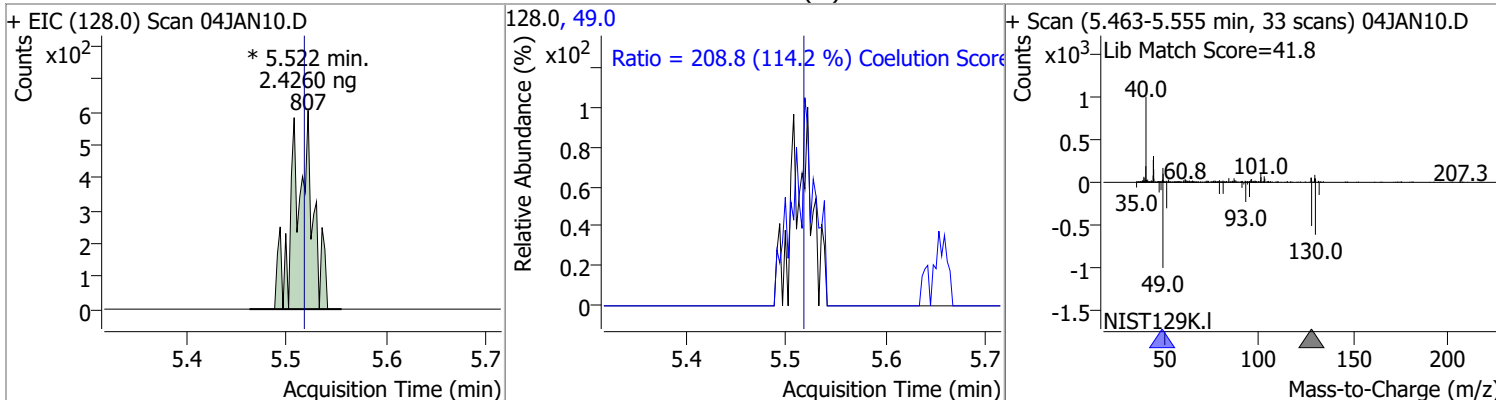


# Quantitation Results Report (QT Reviewed)


| Compound   | Conc.  | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|--------|------|----------|-------|------|--------|-------|-------|
| Chloroform | 2.8946 | 5.66 | 0.01     | 4248  | 85.0 | 63.8   | 36.0  | 96.0  |

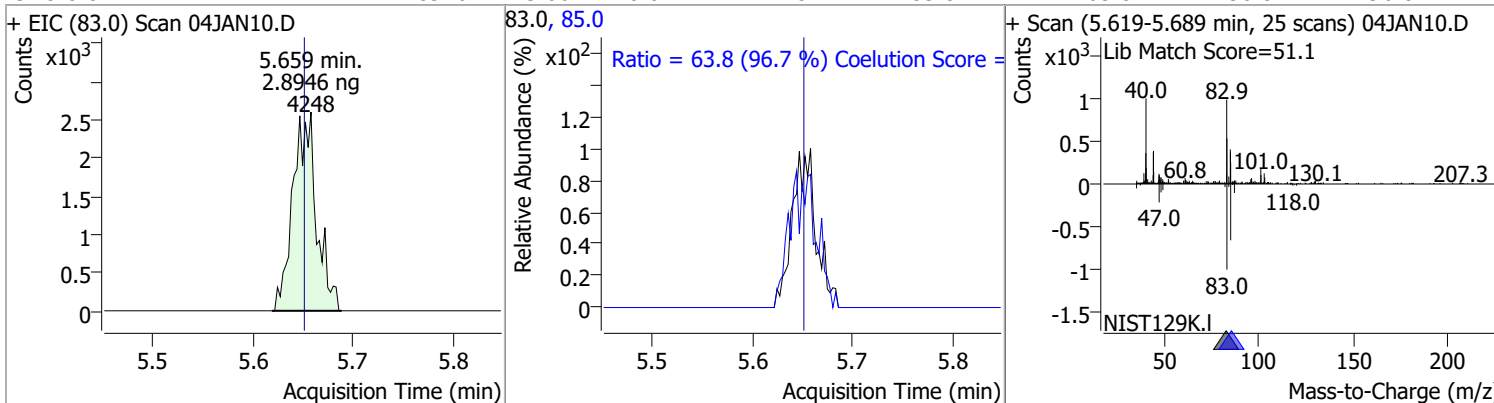


| Compound              | Conc.  | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|--------|------|----------|-------|------|--------|-------|-------|
| 1,1,1-Trichloroethane | 2.5521 | 5.83 | 0.00     | 3510  | 99.0 | 65.9   | 34.7  | 94.7  |
|                       |        |      |          |       | 61.0 | 48.6   | 18.1  | 78.1  |



| Compound             | Conc.  | RT   | Dev(Min) | Resp.    | QIon  | QRatio | Lower | Upper |
|----------------------|--------|------|----------|----------|-------|--------|-------|-------|
| Dibromofluoromethane | 3.4533 | 5.85 | 0.01     | 2508 (m) | 191.5 | 19.1   | 0.0   | 53.1  |

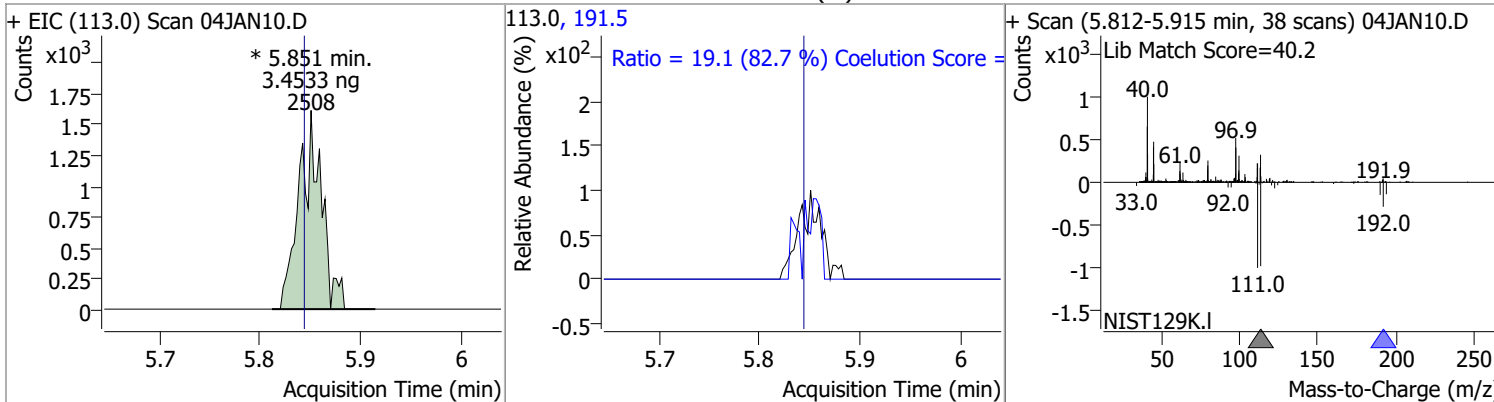


| Compound             | Conc.  | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|----------------------|--------|------|----------|-------|-------|--------|-------|-------|
| Carbon tetrachloride | 3.2043 | 6.03 | 0.01     | 4342  | 119.0 | 72.7   | 67.2  | 127.2 |
|                      |        |      |          |       | 121.0 | 20.8   | 0.1   | 60.1  |

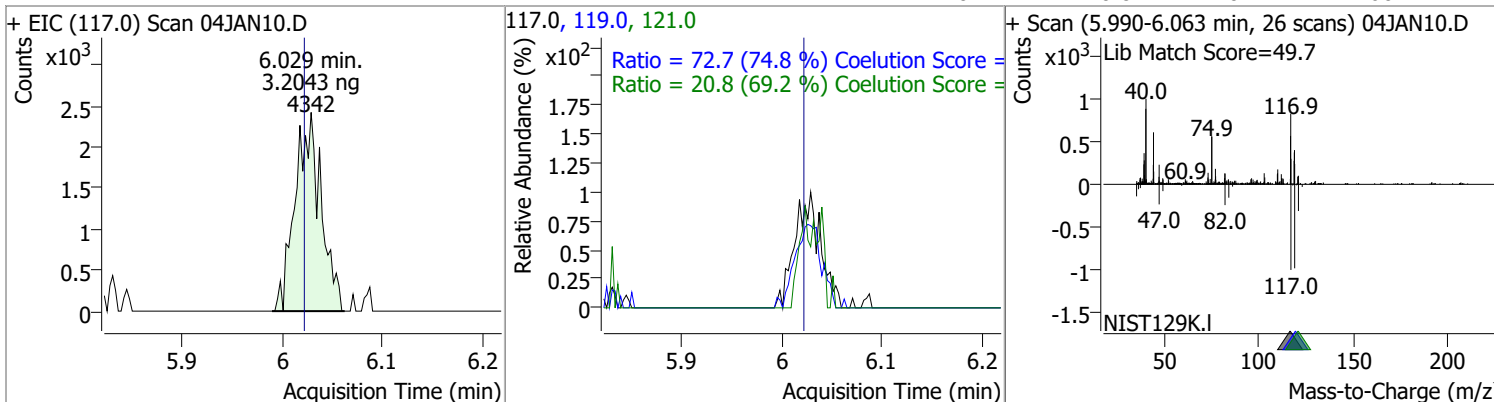


# Quantitation Results Report (QT Reviewed)


| Compound            | Conc.  | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|---------------------|--------|------|----------|-------|-------|--------|-------|-------|
| 1,1-Dichloropropene | 2.4201 | 6.04 | 0.00     | 2830  | 110.0 | 39.7   | 5.9   | 65.9  |
|                     |        |      |          |       | 77.0  | 37.2   | 0.1   | 60.1  |

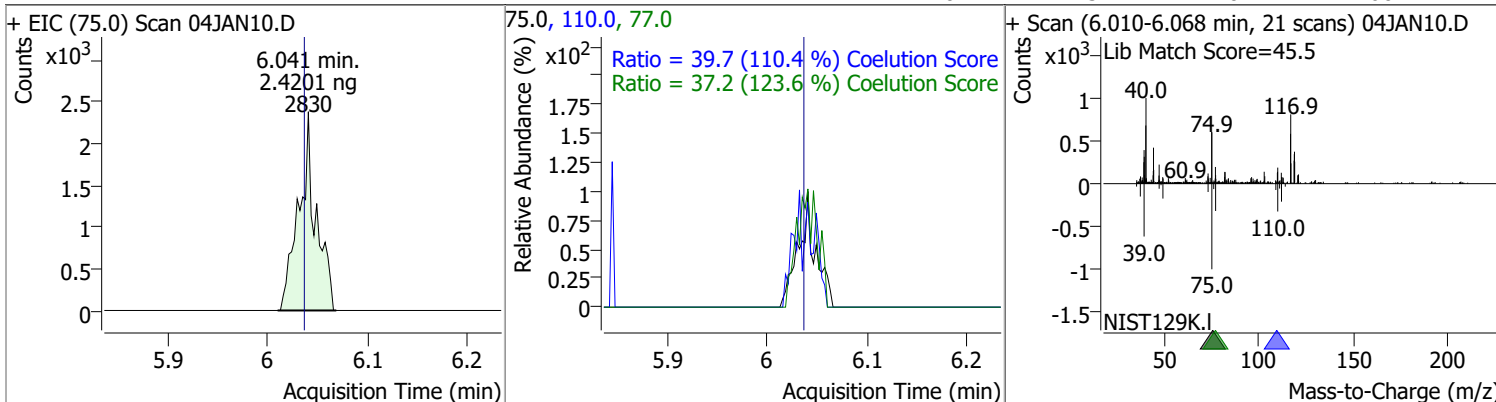


| Compound              | Conc.  | RT   | Dev(Min) | Resp.   | QIon | QRatio | Lower | Upper |
|-----------------------|--------|------|----------|---------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 2.9438 | 6.23 | 0.00     | 923 (m) | 65.0 | 208.6  | 166.5 | 226.5 |

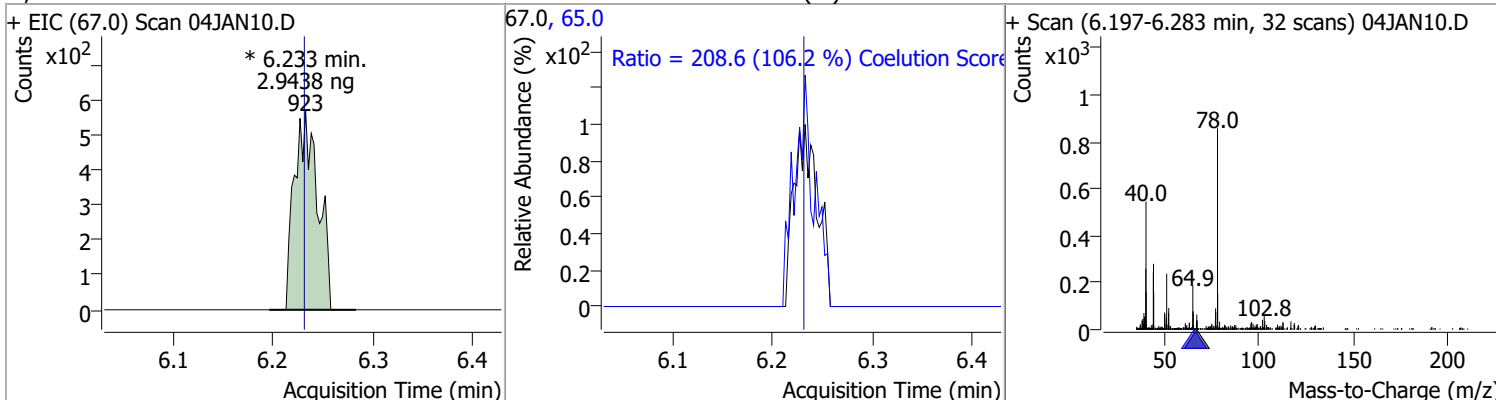

| Compound | Conc.  | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|--------|------|----------|-------|------|--------|-------|-------|
| Benzene  | 2.7393 | 6.28 | 0.00     | 8408  | 77.0 | 22.4   | 0.0   | 53.5  |

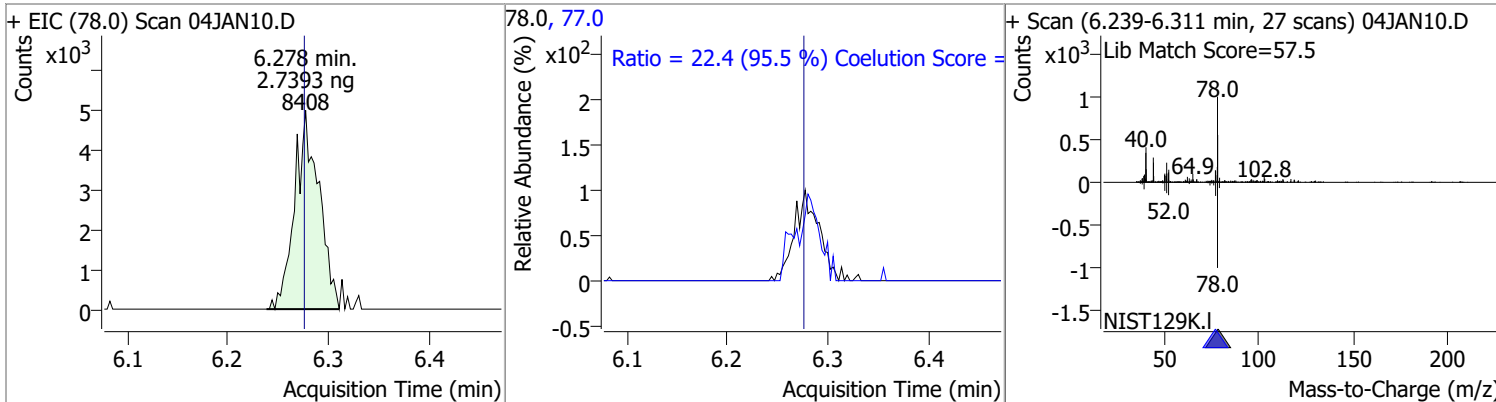


| Compound           | Conc.  | RT   | Dev(Min) | Resp.    | QIon | QRatio | Lower | Upper |
|--------------------|--------|------|----------|----------|------|--------|-------|-------|
| 1,2-Dichloroethane | 2.9090 | 6.32 | 0.00     | 2415 (m) | 64.0 | 31.5   | 0.0   | 59.9  |
|                    |        |      |          |          | 98.0 | 4.9    | 0.0   | 37.6  |

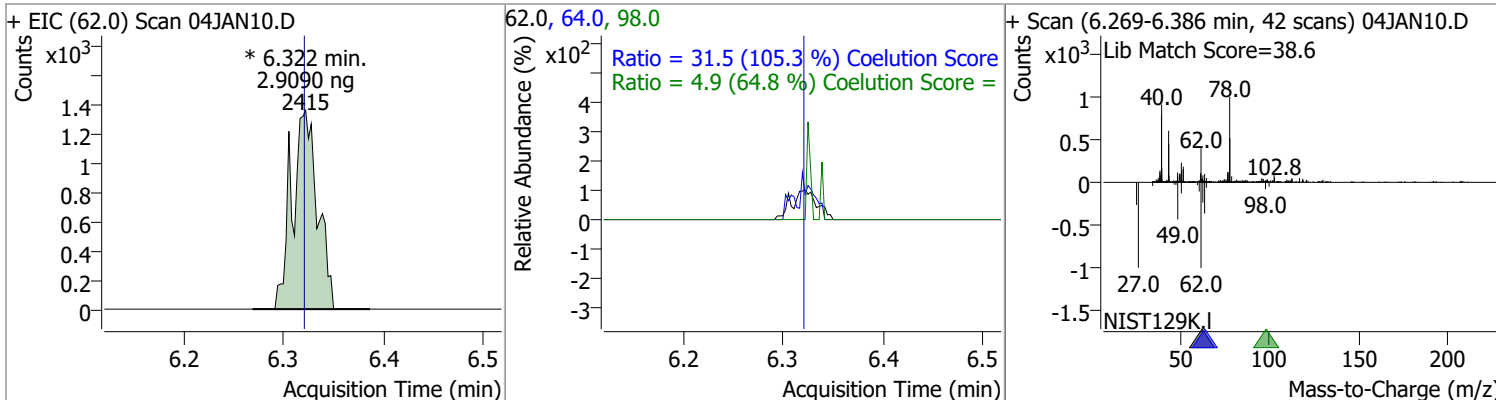




# Quantitation Results Report (QT Reviewed)


| Compound        | Conc.  | RT   | Dev(Min) | Resp.    | QIon  | QRatio | Lower | Upper |
|-----------------|--------|------|----------|----------|-------|--------|-------|-------|
| Trichloroethene | 2.6564 | 7.03 | 0.00     | 2372 (m) | 130.0 | 108.2  | 71.5  | 131.5 |
|                 |        |      |          |          | 97.0  | 69.9   | 34.1  | 94.1  |



| Compound            | Conc.  | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|--------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloropropane | 2.7347 | 7.27 | 0.00     | 2148  | 76.0 | 34.1   | 8.2   | 68.2  |




| Compound       | Conc.  | RT   | Dev(Min) | Resp.   | QIon  | QRatio | Lower | Upper |
|----------------|--------|------|----------|---------|-------|--------|-------|-------|
| Dibromomethane | 2.7162 | 7.40 | 0.00     | 902 (m) | 173.5 | 111.2  | 83.7  | 143.7 |
|                |        |      |          |         | 95.0  | 59.4   | 52.2  | 112.2 |




# Quantitation Results Report (QT Reviewed)


| Compound             | Conc.  | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|----------------------|--------|------|----------|-------|-------|--------|-------|-------|
| Bromodichloromethane | 2.7684 | 7.60 | 0.01     | 2536  | 85.0  | 64.3   | 34.5  | 94.5  |
|                      |        |      |          |       | 127.0 | 5.1    | 0.0   | 39.6  |

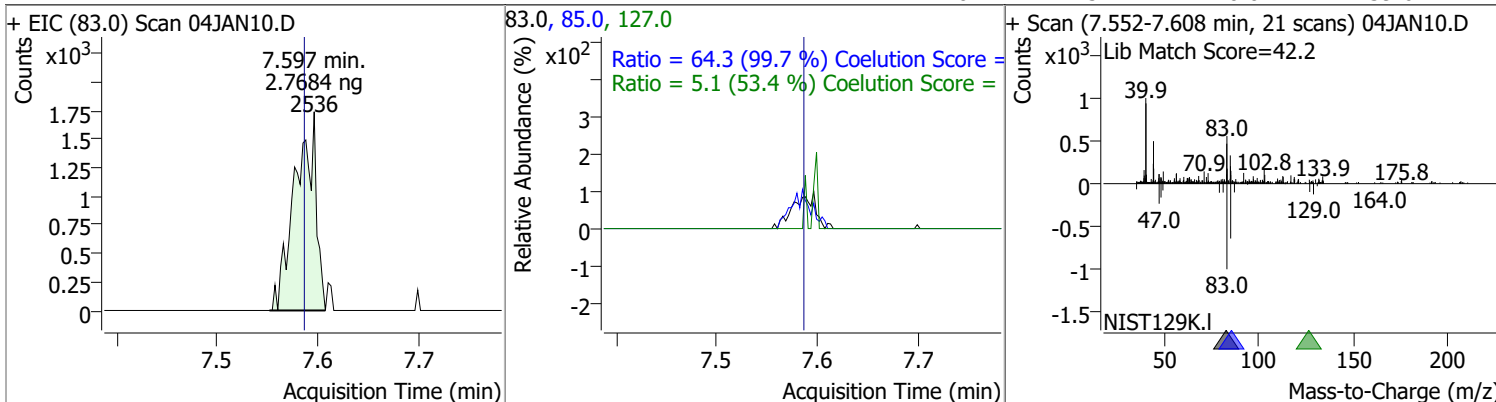

| Compound                | Conc.  | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------------|--------|------|----------|-------|------|--------|-------|-------|
| cis-1,3-Dichloropropene | 2.4939 | 8.05 | -0.01    | 2583  | 39.0 | 56.5   | 23.3  | 83.3  |
|                         |        |      |          |       | 77.0 | 35.7   | 1.0   | 61.0  |

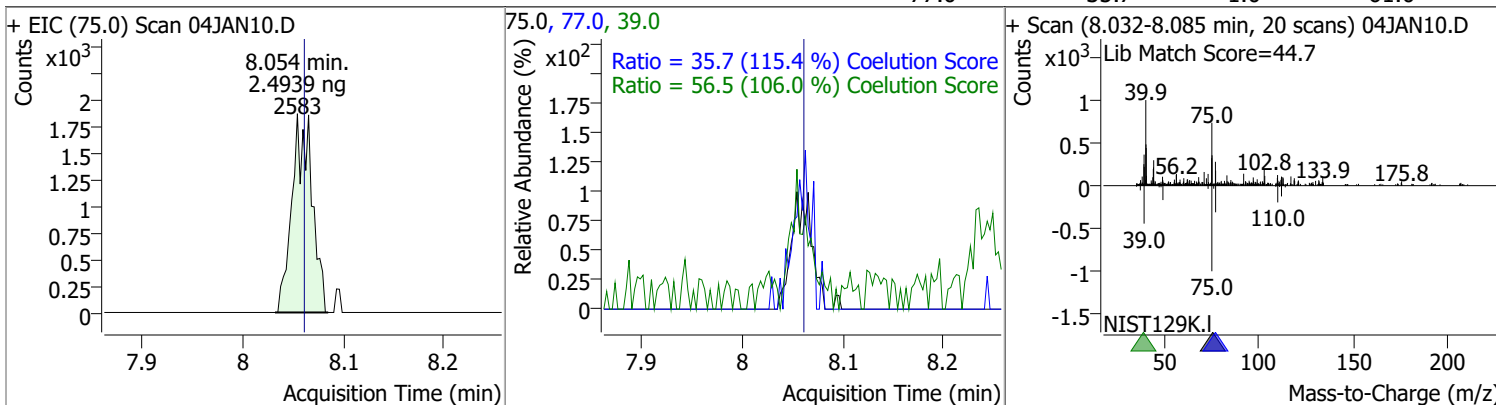


| Compound   | Conc.  | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|------------|--------|------|----------|-------|-------|--------|-------|-------|
| Toluene-d8 | 2.7257 | 8.32 | 0.00     | 7777  | 100.0 | 67.9   | 34.4  | 94.4  |
|            |        |      |          |       | 99.0  | 9.0    | 0.0   | 39.6  |

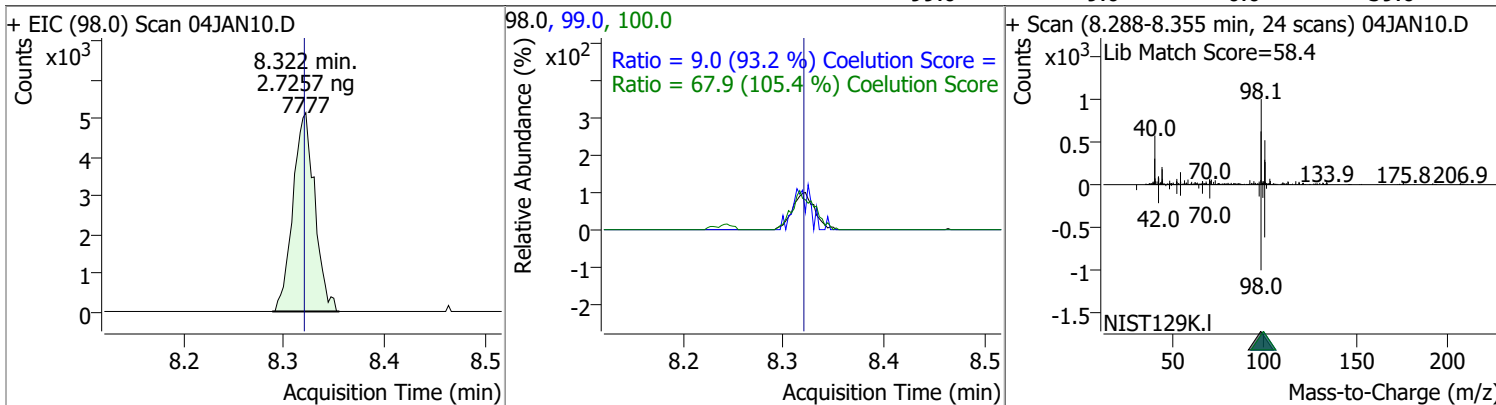


# Quantitation Results Report (QT Reviewed)


| Compound | Conc.  | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|--------|------|----------|-------|------|--------|-------|-------|
| Toluene  | 2.6145 | 8.38 | -0.01    | 5039  | 91.0 | 166.3  | 145.8 | 205.8 |



| Compound                  | Conc.  | RT   | Dev(Min) | Resp.    | QIon | QRatio | Lower | Upper |
|---------------------------|--------|------|----------|----------|------|--------|-------|-------|
| trans-1,3-Dichloropropene | 1.9942 | 8.63 | 0.00     | 1470 (m) | 39.0 | 68.0   | 23.4  | 83.4  |
|                           |        |      |          |          | 77.0 | 38.7   | 2.4   | 62.4  |




| Compound              | Conc.  | RT   | Dev(Min) | Resp.   | QIon | QRatio | Lower | Upper |
|-----------------------|--------|------|----------|---------|------|--------|-------|-------|
| 1,1,2-Trichloroethane | 2.5012 | 8.81 | -0.01    | 960 (m) | 97.0 | 114.4  | 84.6  | 144.6 |
|                       |        |      |          |         | 85.0 | 43.5   | 37.6  | 97.6  |




# Quantitation Results Report (QT Reviewed)


| Compound          | Conc.  | RT   | Dev(Min) | Resp.    | QIon  | QRatio | Lower | Upper |
|-------------------|--------|------|----------|----------|-------|--------|-------|-------|
| Tetrachloroethene | 2.6772 | 8.93 | 0.00     | 2105 (m) | 165.8 | 135.5  | 98.6  | 158.6 |
|                   |        |      |          |          | 129.0 | 95.3   | 61.5  | 121.5 |

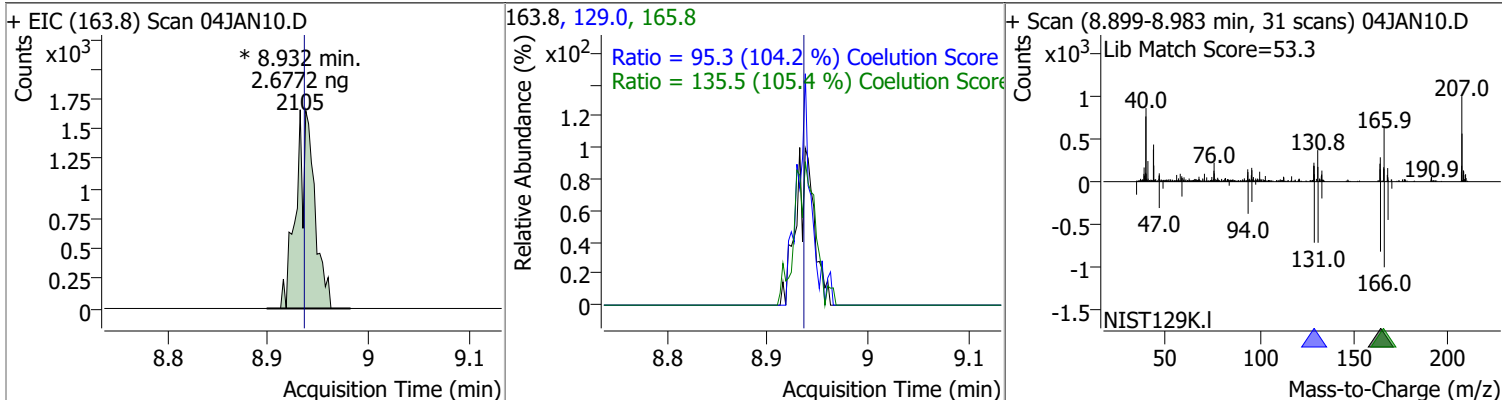


| Compound            | Conc.  | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|--------|------|----------|-------|------|--------|-------|-------|
| 1,3-Dichloropropane | 2.9881 | 8.98 | 0.00     | 2257  | 78.0 | 20.0   | 2.9   | 62.9  |

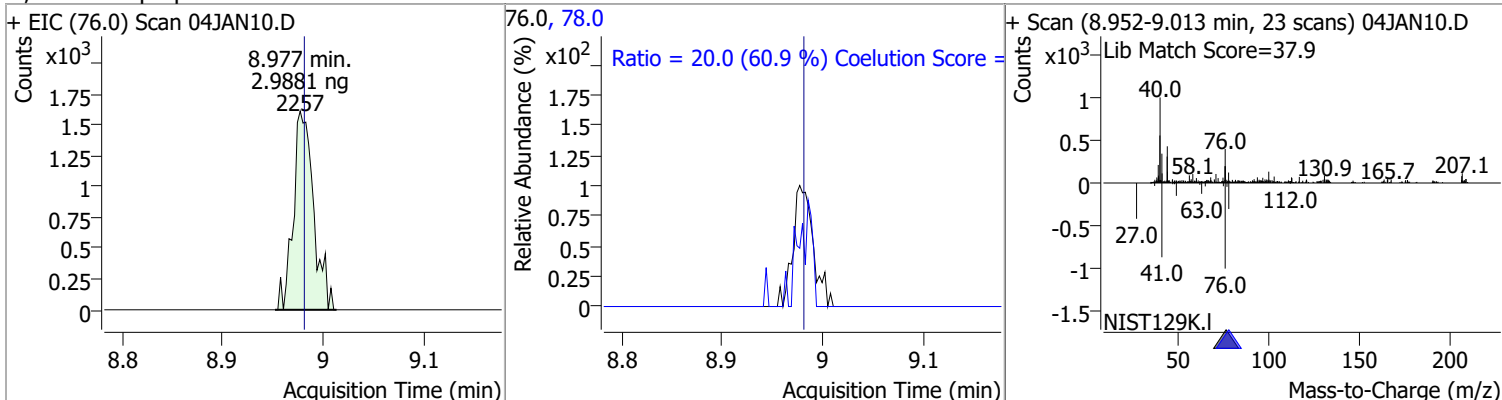

| Compound             | Conc.  | RT   | Dev(Min) | Resp.    | QIon  | QRatio | Lower | Upper |
|----------------------|--------|------|----------|----------|-------|--------|-------|-------|
| Chlorodibromomethane | 2.4461 | 9.20 | 0.00     | 1468 (m) | 127.0 | 77.7   | 48.0  | 108.0 |

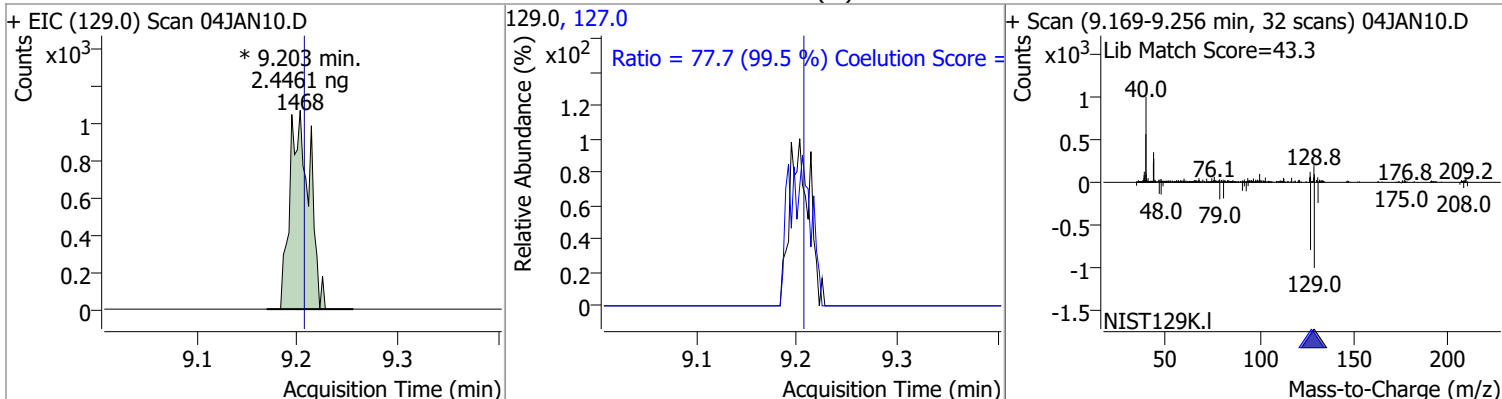


| Compound          | Conc.  | RT   | Dev(Min) | Resp.    | QIon  | QRatio | Lower | Upper |
|-------------------|--------|------|----------|----------|-------|--------|-------|-------|
| 1,2-Dibromoethane | 3.0943 | 9.30 | -0.01    | 1299 (m) | 109.0 | 80.0   | 64.5  | 124.5 |

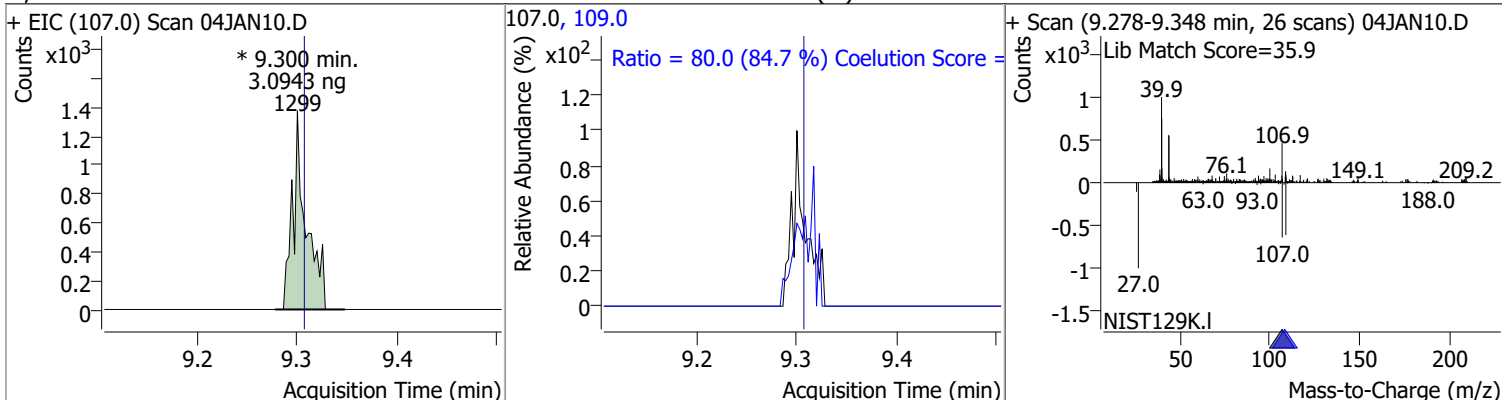


# Quantitation Results Report (QT Reviewed)


| Compound      | Conc.  | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|---------------|--------|------|----------|-------|-------|--------|-------|-------|
| Chlorobenzene | 2.7350 | 9.81 | 0.00     | 5771  | 114.0 | 32.2   | 2.1   | 62.1  |




| Compound                  | Conc.  | RT   | Dev(Min) | Resp.    | QIon  | QRatio | Lower | Upper |
|---------------------------|--------|------|----------|----------|-------|--------|-------|-------|
| 1,1,1,2-Tetrachloroethane | 2.5659 | 9.89 | 0.00     | 1893 (m) | 133.0 | 101.0  | 68.6  | 128.6 |







| Compound     | Conc.  | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|--------------|--------|------|----------|-------|-------|--------|-------|-------|
| Ethylbenzene | 2.5367 | 9.92 | 0.00     | 9283  | 106.0 | 35.2   | 1.1   | 61.1  |



| Compound    | Conc.  | RT    | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------|--------|-------|----------|-------|------|--------|-------|-------|
| m+p-Xylenes | 5.0712 | 10.05 | 0.01     | 7212  | 91.0 | 183.3  | 171.4 | 231.4 |




# Quantitation Results Report (QT Reviewed)




# Quantitation Results Report (QT Reviewed)


| Compound     | Conc.  | RT    | Dev(Min) | Resp.    | QIon  | QRatio | Lower | Upper |
|--------------|--------|-------|----------|----------|-------|--------|-------|-------|
| Bromobenzene | 2.7439 | 11.09 | -0.01    | 2024 (m) | 77.0  | 134.0  | 115.7 | 175.7 |
|              |        |       |          |          | 158.0 | 95.6   | 66.5  | 126.5 |

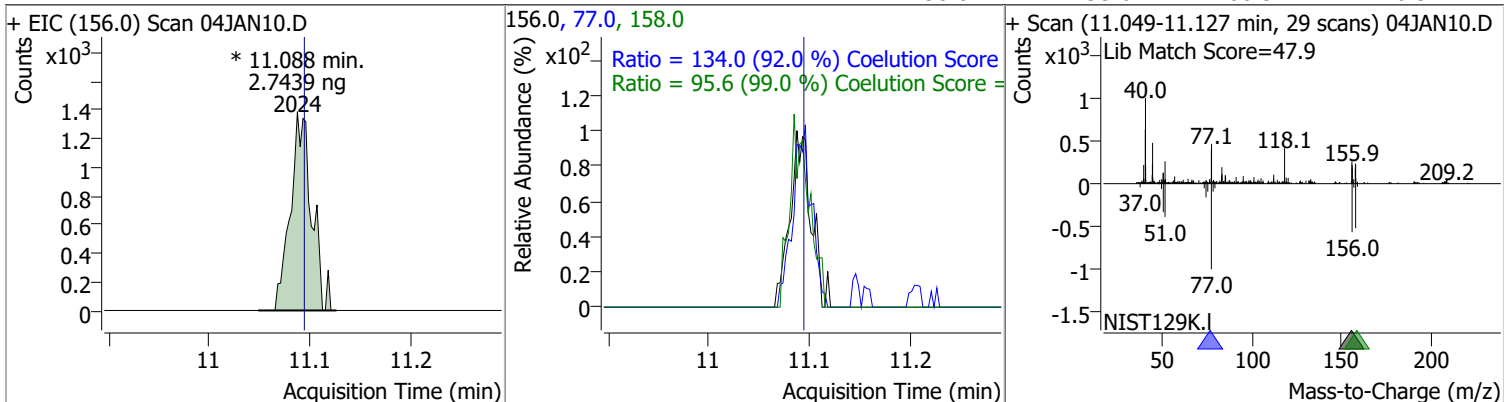


| Compound                  | Conc.  | RT    | Dev(Min) | Resp.    | QIon | QRatio | Lower | Upper |
|---------------------------|--------|-------|----------|----------|------|--------|-------|-------|
| 1,1,2,2-Tetrachloroethane | 2.6916 | 11.11 | 0.00     | 1142 (m) | 85.0 | 73.0   | 36.2  | 96.2  |

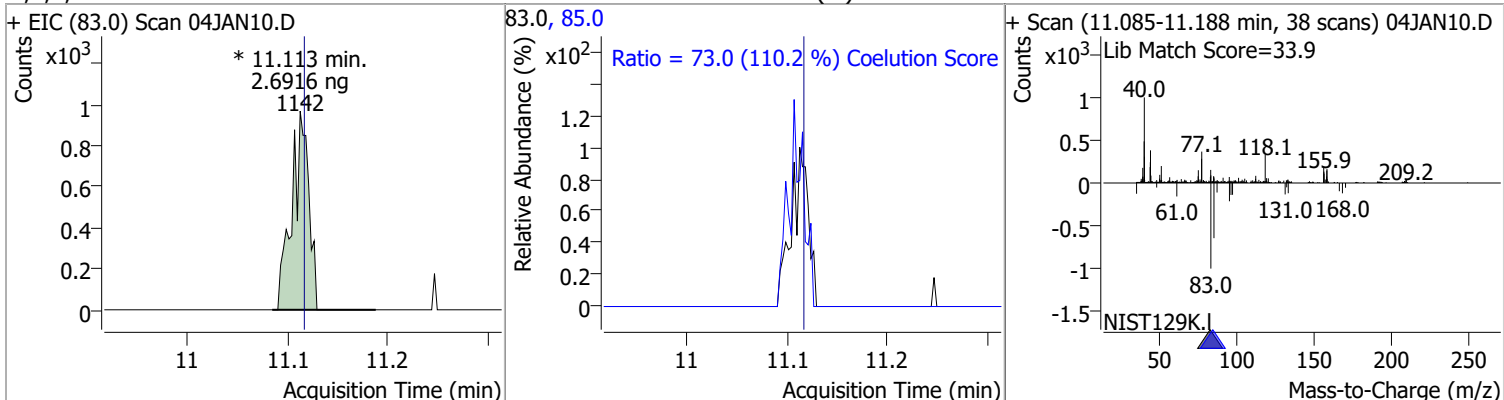

| Compound               | Conc. | Exp RT | QIon  | Exp Ratio |
|------------------------|-------|--------|-------|-----------|
| 1,2,3-Trichloropropane | N.D.  | 11.15  | 112.0 | 63.5      |



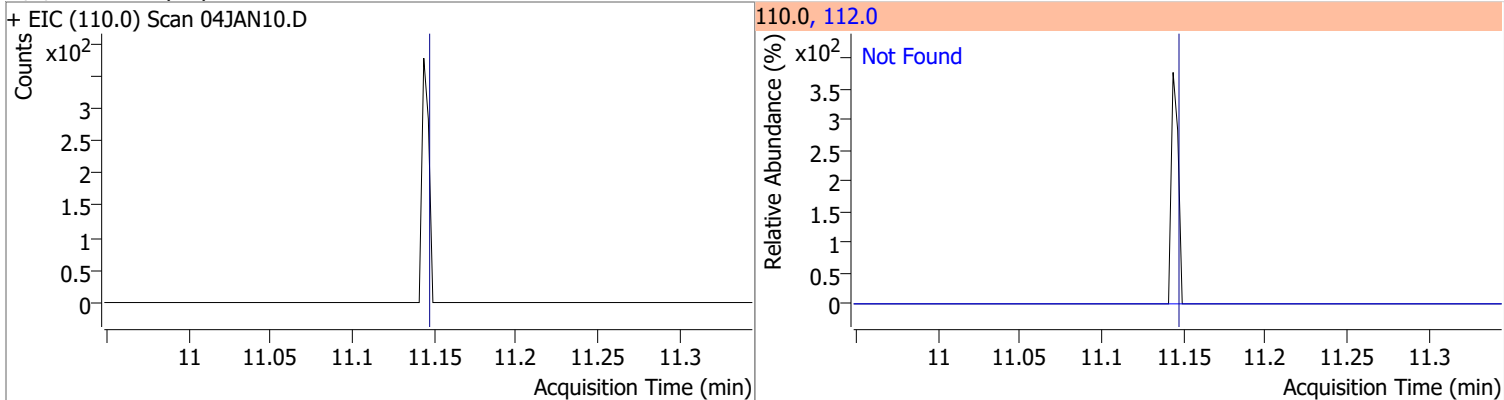


| Compound        | Conc.  | RT    | Dev(Min) | Resp.    | QIon | QRatio | Lower | Upper |
|-----------------|--------|-------|----------|----------|------|--------|-------|-------|
| 2-Chlorotoluene | 2.5124 | 11.29 | 0.00     | 1844 (m) | 91.0 | 288.1  | 252.3 | 312.3 |



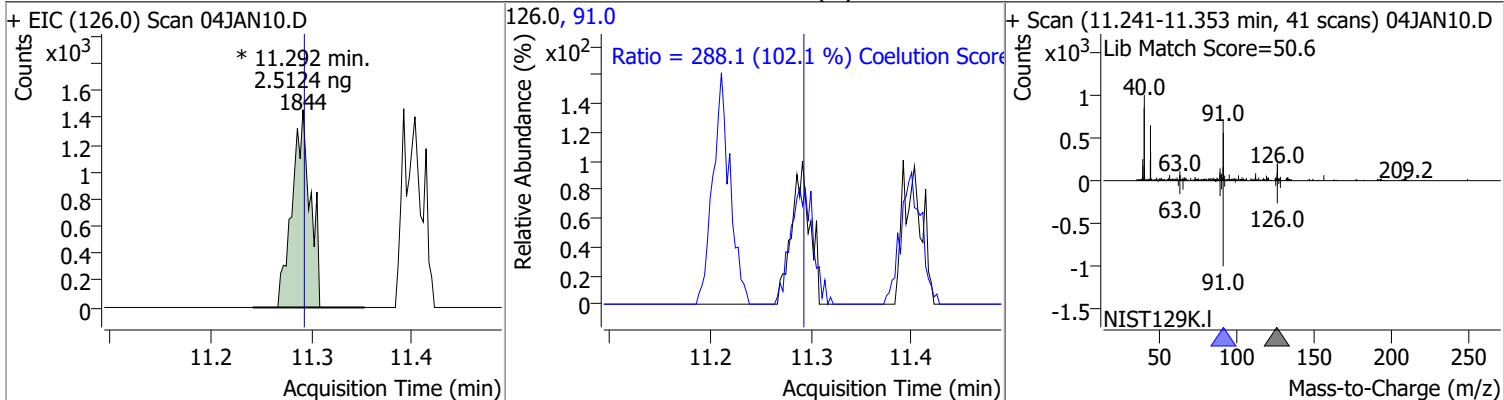


# Quantitation Results Report (QT Reviewed)




| Compound        | Conc.  | RT    | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|-----------------|--------|-------|----------|-------|-------|--------|-------|-------|
| 4-Chlorotoluene | 2.2650 | 11.40 | 0.00     | 5419  | 126.0 | 33.9   | 1.7   | 61.7  |

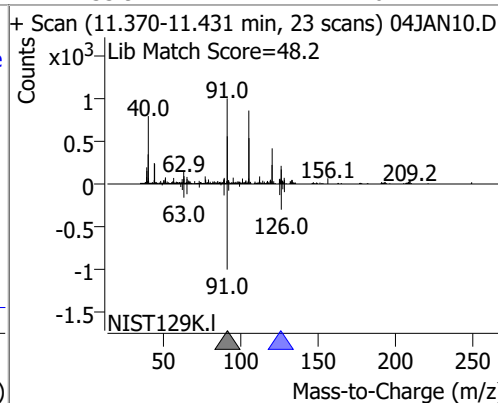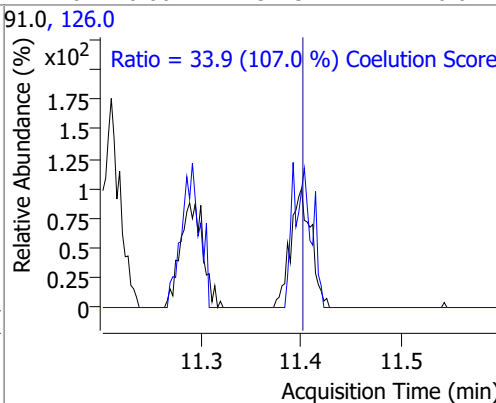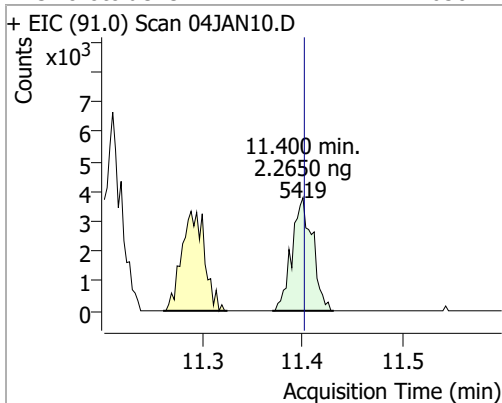

| Compound            | Conc.  | RT    | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|---------------------|--------|-------|----------|-------|-------|--------|-------|-------|
| 1,3-Dichlorobenzene | 2.6327 | 12.03 | 0.00     | 3541  | 148.0 | 63.6   | 33.6  | 93.6  |
|                     |        |       |          |       | 111.0 | 41.5   | 9.8   | 69.8  |

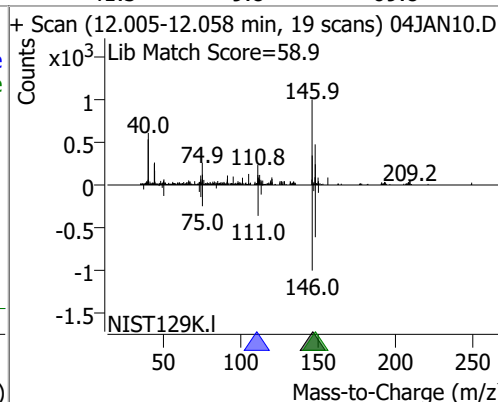




| Compound            | Conc.  | RT    | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|---------------------|--------|-------|----------|-------|-------|--------|-------|-------|
| 1,4-Dichlorobenzene | 2.7613 | 12.13 | 0.00     | 3787  | 148.0 | 66.5   | 33.1  | 93.1  |
|                     |        |       |          |       | 111.0 | 28.2   | 9.1   | 69.1  |

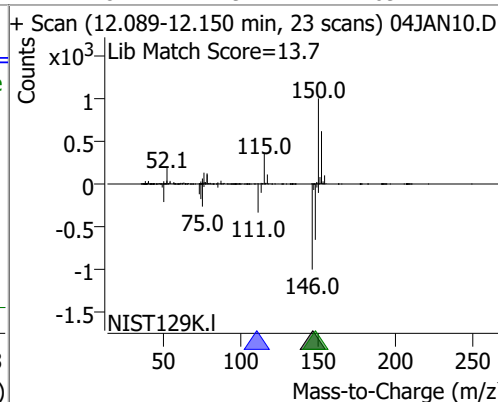




# Quantitation Results Report (QT Reviewed)

| Compound            | Conc.  | RT    | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|---------------------|--------|-------|----------|-------|-------|--------|-------|-------|
| 1,2-Dichlorobenzene | 2.7307 | 12.50 | 0.01     | 3104  | 148.0 | 61.0   | 33.9  | 93.9  |
|                     |        |       |          |       | 111.0 | 38.4   | 11.0  | 71.0  |

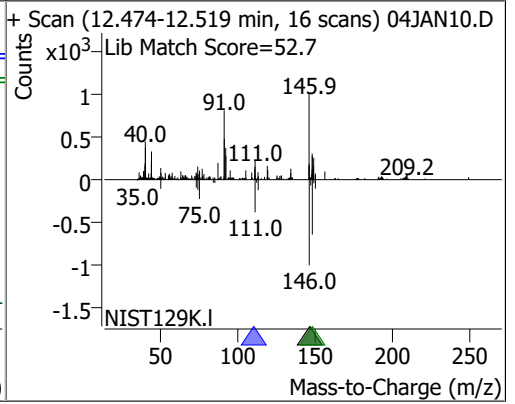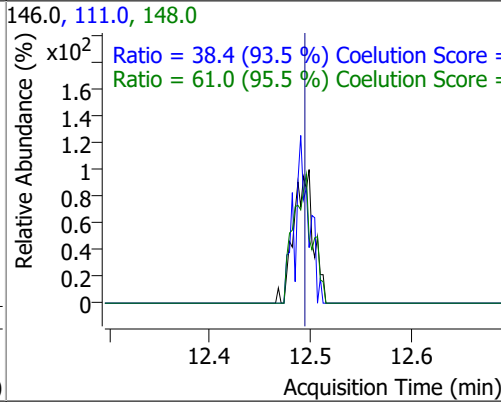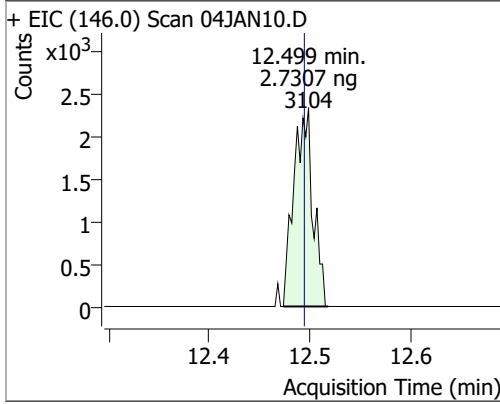

# Quantitation Results Report (QT Reviewed)

|                |                                     |                   |                       |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File      | 04JAN11.D                           | Operator          | MSC                   |
| Acq. Method    | 5975CACQF.M                         | Acq. Date-Time    | 1/4/2022 4:00:35 PM   |
| Sample Name    | ICAL010422_2                        | Instrument        | VOA5975C              |
| Vial           | 11                                  | Multiplier        | 1.00                  |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m  | Comment           |                       |
| Tune File      | BFB_Atune3.u                        | Tune Date         | 10/11/2021 4:02:00 PM |
| Batch Name     | VG010422_8260B.batch.bin            | Last Calib Update | 1/9/2022 8:59:52 PM   |
| Ref Library    | \\MASSHUNTER\Org\Library\NIST129K.I |                   |                       |















| Compound                           | RT                   | QIon  | Resp.  | Conc.            | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|------------------|-------|----------|
| <b>Internal Standards</b>          |                      |       |        |                  |       |          |
| M Fluorobenzene                    | 6.621                | 96.0  | 764419 | 250.0000         | ng    | -0.003   |
| M Chlorobenzene-d5                 | 9.774                | 82.0  | 296554 | 250.0000         | ng    | 0.003    |
| M 1,4-Dichlorobenzene-d4           | 12.103               | 152.0 | 242142 | 250.0000         | ng    | 0.003    |
| <b>System Monitoring Compounds</b> |                      |       |        |                  |       |          |
| S Dibromofluoromethane             | 5.845                | 113.0 | 9074   | 12.6000          | ng    | 0.000    |
| Spiked Amount: 250.000             | Range: 80.0 - 119.0% |       |        | Recovery = 5.04% | *     |          |
| S 1,2-Dichloroethane-d4            | 6.227                | 67.0  | 3938   | 12.6600          | ng    | -0.006   |
| Spiked Amount: 250.000             | Range: 81.0 - 118.0% |       |        | Recovery = 5.06% | *     |          |
| S Toluene-d8                       | 8.322                | 98.0  | 32318  | 11.3089          | ng    | 0.003    |
| Spiked Amount: 250.000             | Range: 89.0 - 112.0% |       |        | Recovery = 4.52% | *     |          |
| S p-Bromofluorobenzene             | 10.948               | 95.0  | 10059  | 11.3393          | ng    | -0.006   |
| Spiked Amount: 250.000             | Range: 85.0 - 114.0% |       |        | Recovery = 4.54% | *     |          |
| <b>Target Compounds</b>            |                      |       |        |                  |       |          |
| T Dichlorodifluoromethane          | 1.244                | 85.0  | 12087  | 12.0663          | ng    | 96       |
| T Chloromethane                    | 1.406                | 50.0  | 16859  | 13.8661          | ng    | 100      |
| T Vinyl chloride                   | 1.498                | 62.0  | 13724  | 12.5446          | ng    | 75       |
| T Bromomethane                     | 1.796                | 96.0  | 5893   | 12.0464          | ng    | 97       |
| T Chloroethane                     | 1.897                | 64.0  | 8052   | 14.8670          | ng    | m 98     |
| T Trichlorofluoromethane           | 2.142                | 101.0 | 15431  | 11.3637          | ng    | 95       |
| T 1,1-Dichloroethene               | 2.700                | 96.0  | 9169   | 11.9081          | ng    | 96       |
| T Methylene chloride               | 3.338                | 49.0  | 17734  | 15.6236          | ng    | 93       |
| T trans-1,2-Dichloroethene         | 3.720                | 96.0  | 9821   | 12.5022          | ng    | m 95     |
| T Methyl tert-butyl ether (MTBE)   | 3.762                | 73.0  | 12515  | 12.3255          | ng    | m 99     |
| T 1,1-Dichloroethane               | 4.378                | 63.0  | 17642  | 12.0652          | ng    | 94       |
| T 2,2-Dichloropropane              | 5.196                | 77.0  | 13676  | 12.4820          | ng    | 95       |
| T cis-1,2-Dichloroethene           | 5.221                | 96.0  | 10008  | 12.5659          | ng    | 95       |
| T Methyl ethyl ketone              | 5.288                | 43.0  | 13167  | 122.0520         | ng    | 95       |
| T Bromochloromethane               | 5.516                | 128.0 | 4275   | 12.9568          | ng    | 91       |
| T Chloroform                       | 5.656                | 83.0  | 19015  | 13.0668          | ng    | 98       |

# Quantitation Results Report (QT Reviewed)





| Compound                    | RT     | QIon  | Resp. | Conc.   | Units | Dev(Min) |
|-----------------------------|--------|-------|-------|---------|-------|----------|
| T 1,1,1-Trichloroethane     | 5.837  | 97.0  | 16623 | 12.1891 | ng    | 97       |
| T Carbon tetrachloride      | 6.021  | 117.0 | 16466 | 12.2545 | ng    | 98       |
| T 1,1-Dichloropropene       | 6.038  | 75.0  | 13149 | 11.3397 | ng    | 94       |
| T Benzene                   | 6.278  | 78.0  | 37071 | 12.1801 | ng    | 99       |
| T 1,2-Dichloroethane        | 6.322  | 62.0  | 10202 | 12.3906 | ng    | 92       |
| T Trichloroethene           | 7.025  | 95.0  | 10442 | 11.6753 | ng    | 94       |
| T 1,2-Dichloropropane       | 7.270  | 63.0  | 9488  | 12.0602 | ng    | 99       |
| T Dibromomethane            | 7.399  | 93.0  | 4675  | 14.0619 | ng    | 93       |
| T Bromodichloromethane      | 7.585  | 83.0  | 11562 | 12.6014 | ng    | 97       |
| T cis-1,3-Dichloropropene   | 8.062  | 75.0  | 12525 | 12.0738 | ng    | 94       |
| T Toluene                   | 8.388  | 92.0  | 21794 | 11.2899 | ng    | 97       |
| T trans-1,3-Dichloropropene | 8.645  | 75.0  | 8683  | 11.7589 | ng    | 98       |
| T 1,1,2-Trichloroethane     | 8.824  | 83.0  | 5090  | 13.2340 | ng    | m 91     |
| T Tetrachloroethene         | 8.935  | 163.8 | 9238  | 11.7302 | ng    | 99       |
| T 1,3-Dichloropropane       | 8.985  | 76.0  | 8967  | 11.8526 | ng    | 97       |
| T Chlorodibromomethane      | 9.206  | 129.0 | 7718  | 12.8393 | ng    | 97       |
| T 1,2-Dibromoethane         | 9.300  | 107.0 | 5410  | 12.8640 | ng    | 100      |
| T Chlorobenzene             | 9.802  | 112.0 | 26461 | 12.5204 | ng    | 99       |
| T 1,1,1,2-Tetrachloroethane | 9.889  | 131.0 | 9473  | 12.8225 | ng    | 88       |
| T Ethylbenzene              | 9.917  | 91.0  | 40470 | 11.0411 | ng    | 99       |
| T m+p-Xylenes               | 10.037 | 106.0 | 31538 | 22.1410 | ng    | 100      |
| T o-Xylene                  | 10.430 | 106.0 | 13519 | 10.6612 | ng    | 92       |
| T Styrene                   | 10.449 | 104.0 | 23472 | 11.4968 | ng    | 100      |
| T Bromoform                 | 10.625 | 172.5 | 3652  | 11.7860 | ng    | 92       |
| T Bromobenzene              | 11.096 | 156.0 | 9663  | 12.3310 | ng    | 96       |
| T 1,1,2,2-Tetrachloroethane | 11.116 | 83.0  | 5793  | 12.8437 | ng    | 99       |
| T 1,2,3-Trichloropropane    | 11.144 | 110.0 | 1654  | 13.7084 | ng    | m 99     |
| T 2-Chlorotoluene           | 11.289 | 126.0 | 8731  | 11.1977 | ng    | 94       |
| T 4-Chlorotoluene           | 11.400 | 91.0  | 28532 | 11.2233 | ng    | 100      |
| T 1,3-Dichlorobenzene       | 12.036 | 146.0 | 16932 | 11.8473 | ng    | 99       |
| T 1,4-Dichlorobenzene       | 12.122 | 146.0 | 17438 | 11.9662 | ng    | 94       |
| T 1,2-Dichlorobenzene       | 12.493 | 146.0 | 14666 | 12.1423 | ng    | 98       |

(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (\*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

# Quantitation Results Report (QT Reviewed)

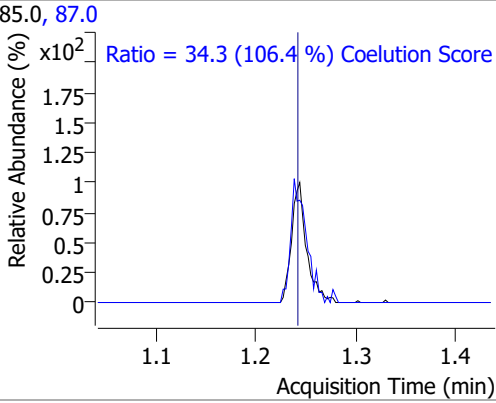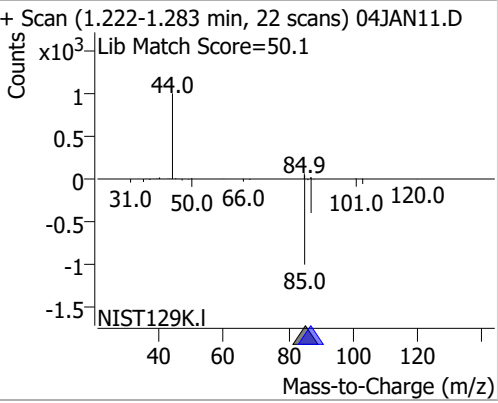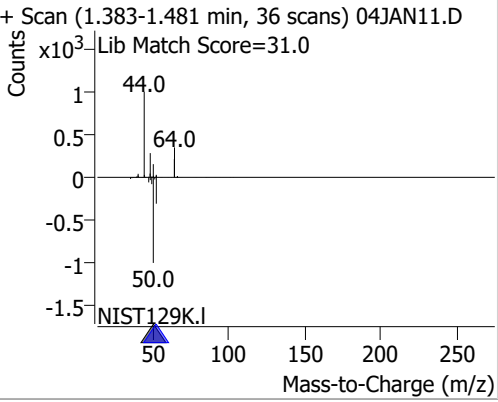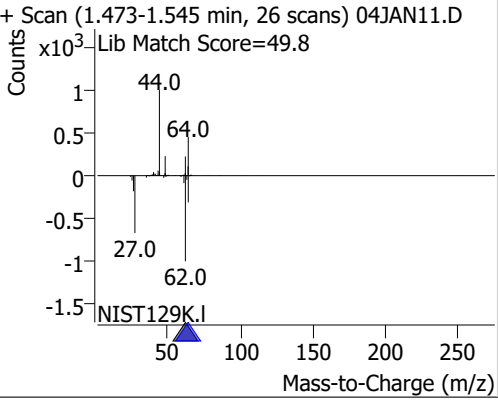
| Compound                                                                           | Conc.                                                                                | RT   | Dev(Min)                               | Resp. | QIon | QRatio                                       | Lower | Upper |                                                                                       |
|------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------|------|----------------------------------------|-------|------|----------------------------------------------|-------|-------|---------------------------------------------------------------------------------------|
| Dichlorodifluoromethane                                                            | 12.0663                                                                              | 1.24 | 0.00                                   | 12087 | 87.0 | 34.3                                         | 2.3   | 62.3  |                                                                                       |
| + EIC (85.0) Scan 04JAN11.D                                                        |                                                                                      |      | 85.0, 87.0                             |       |      | + Scan (1.222-1.283 min, 22 scans) 04JAN11.D |       |       |                                                                                       |
|    |    |      | Ratio = 34.3 (106.4 %) Coelution Score |       |      |                                              |       |       |    |
| Chloromethane                                                                      | 13.8661                                                                              | 1.41 | 0.00                                   | 16859 | 52.0 | 32.0                                         | 2.1   | 62.1  |                                                                                       |
| + EIC (50.0) Scan 04JAN11.D                                                        |                                                                                      |      | 50.0, 52.0                             |       |      | + Scan (1.383-1.481 min, 36 scans) 04JAN11.D |       |       |                                                                                       |
|   |   |      | Ratio = 32.0 (99.5 %) Coelution Score  |       |      |                                              |       |       |   |
| Vinyl chloride                                                                     | 12.5446                                                                              | 1.50 | 0.00                                   | 13724 | 64.0 | 43.5                                         | 0.0   | 59.9  |                                                                                       |
| + EIC (62.0) Scan 04JAN11.D                                                        |                                                                                      |      | 62.0, 64.0                             |       |      | + Scan (1.473-1.545 min, 26 scans) 04JAN11.D |       |       |                                                                                       |
|  |  |      | Ratio = 43.5 (145.5 %) Coelution Score |       |      |                                              |       |       |  |
| Bromomethane                                                                       | 12.0464                                                                              | 1.80 | 0.00                                   | 5893  | 94.0 | 101.9                                        | 74.6  | 134.6 |                                                                                       |
| + EIC (96.0) Scan 04JAN11.D                                                        |                                                                                      |      | 96.0, 94.0                             |       |      | + Scan (1.771-1.838 min, 25 scans) 04JAN11.D |       |       |                                                                                       |
|  |  |      | Ratio = 101.9 (97.4 %) Coelution Score |       |      |                                              |       |       |  |

# Quantitation Results Report (QT Reviewed)




# Quantitation Results Report (QT Reviewed)


| Compound                 | Conc.   | RT   | Dev(Min) | Resp.    | QIon | QRatio | Lower | Upper |
|--------------------------|---------|------|----------|----------|------|--------|-------|-------|
| trans-1,2-Dichloroethene | 12.5022 | 3.72 | 0.00     | 9821 (m) | 61.0 | 146.7  | 123.9 | 183.9 |
|                          |         |      |          |          | 98.0 | 63.0   | 35.7  | 95.7  |



| Compound                       | Conc.   | RT   | Dev(Min) | Resp.     | QIon | QRatio | Lower | Upper |
|--------------------------------|---------|------|----------|-----------|------|--------|-------|-------|
| Methyl tert-butyl ether (MTBE) | 12.3255 | 3.76 | 0.01     | 12515 (m) | 57.0 | 24.3   | 0.0   | 54.6  |




| Compound           | Conc.   | RT   | Dev(Min) | Resp.     | QIon | QRatio | Lower | Upper |
|--------------------|---------|------|----------|-----------|------|--------|-------|-------|
| 1,1-Dichloroethane | 12.0652 | 4.38 | 0.00     | 17642 (m) | 65.0 | 35.8   | 2.1   | 62.1  |
|                    |         |      |          |           | 83.0 | 15.3   | 0.0   | 43.7  |




# Quantitation Results Report (QT Reviewed)


| Compound            | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|---------|------|----------|-------|------|--------|-------|-------|
| 2,2-Dichloropropane | 12.4820 | 5.20 | 0.00     | 13676 | 41.0 | 69.9   | 36.5  | 96.5  |
|                     |         |      |          |       | 97.0 | 27.3   | 0.0   | 53.2  |

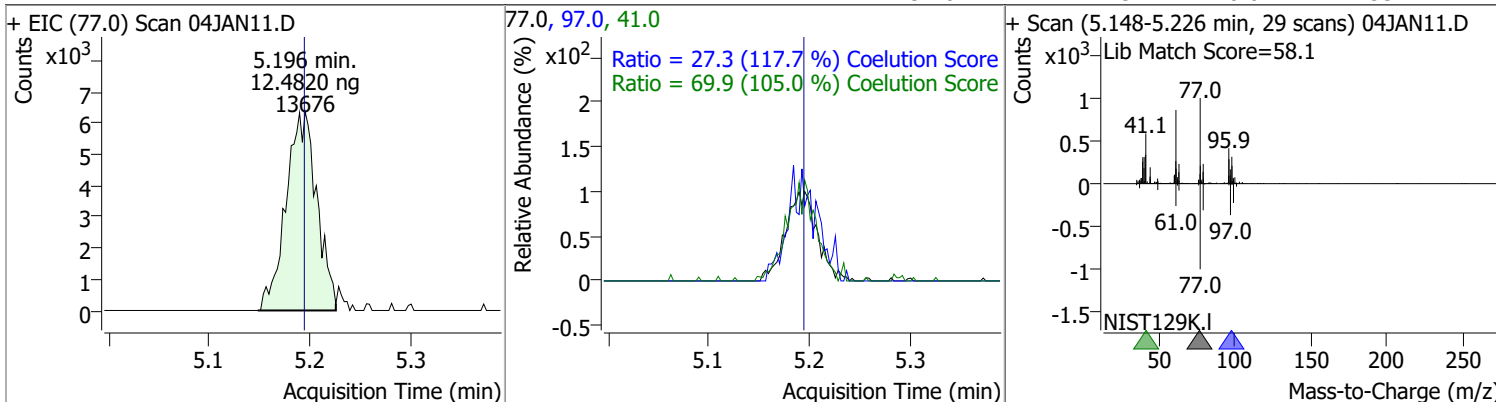


| Compound               | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|---------|------|----------|-------|------|--------|-------|-------|
| cis-1,2-Dichloroethene | 12.5659 | 5.22 | 0.01     | 10008 | 61.0 | 158.3  | 137.2 | 197.2 |
|                        |         |      |          |       | 98.0 | 68.8   | 37.3  | 97.3  |

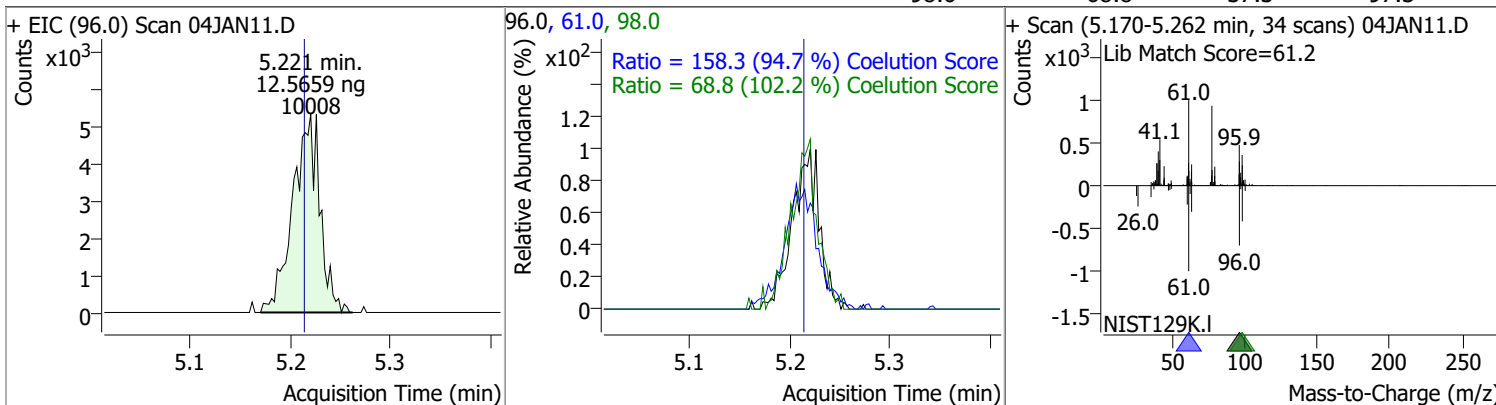





| Compound            | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|-------|------|--------|-------|-------|
| Methyl ethyl ketone | 122.0520 | 5.29 | 0.01     | 13167 | 72.0 | 18.8   | 0.0   | 51.3  |

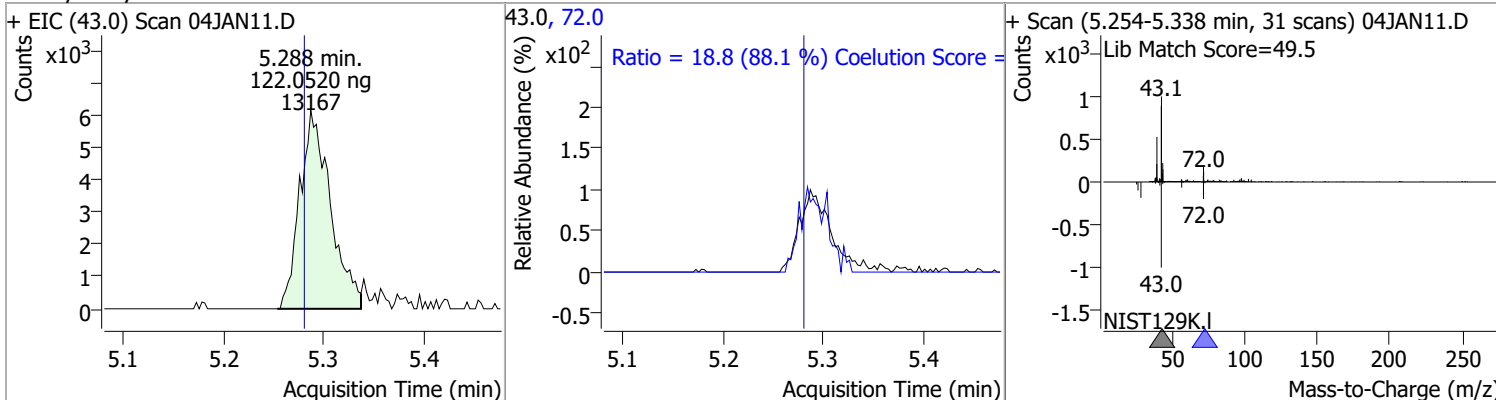

| Compound           | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|---------|------|----------|-------|------|--------|-------|-------|
| Bromochloromethane | 12.9568 | 5.52 | 0.00     | 4275  | 49.0 | 169.7  | 152.9 | 212.9 |












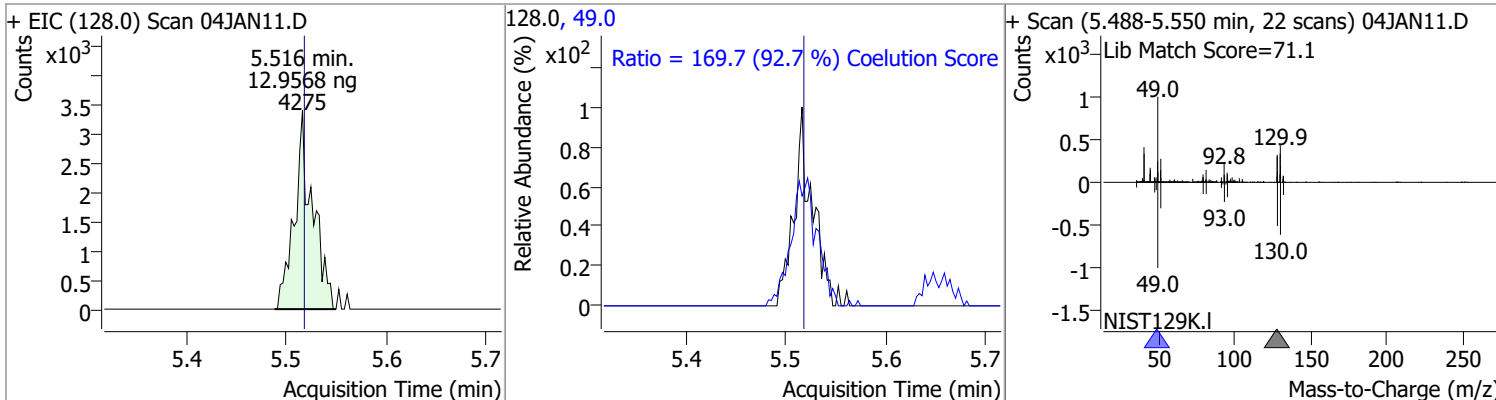


# Quantitation Results Report (QT Reviewed)

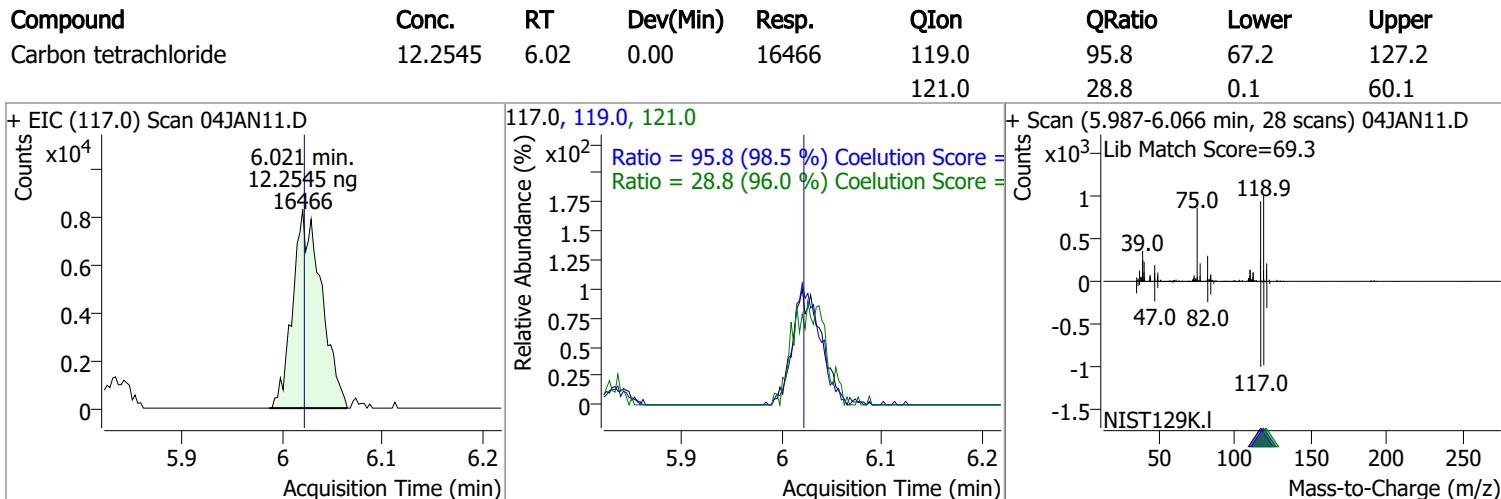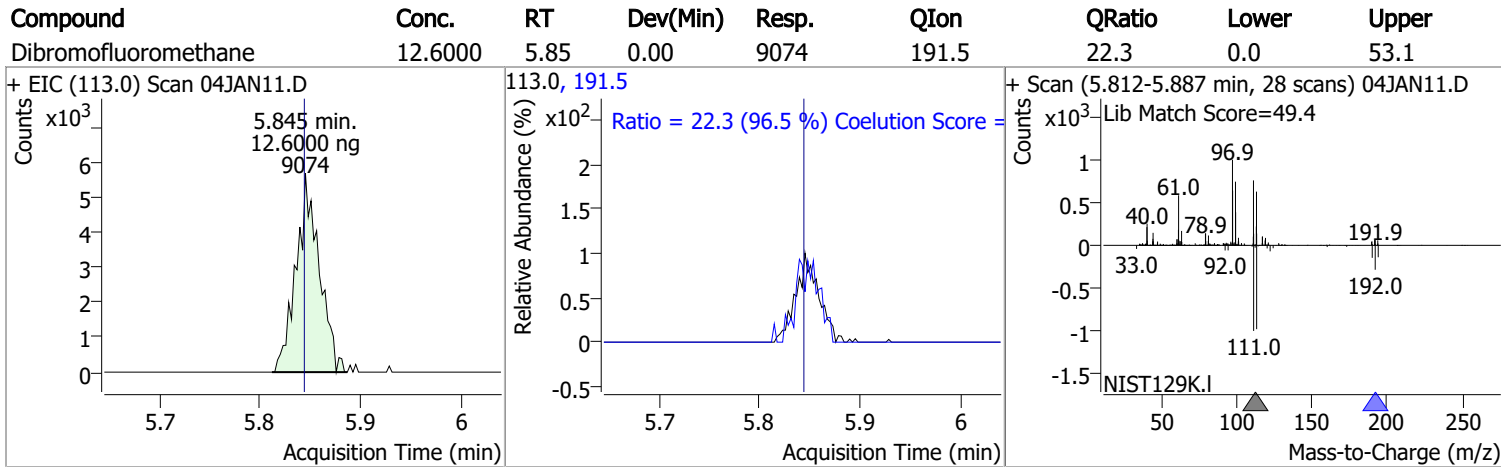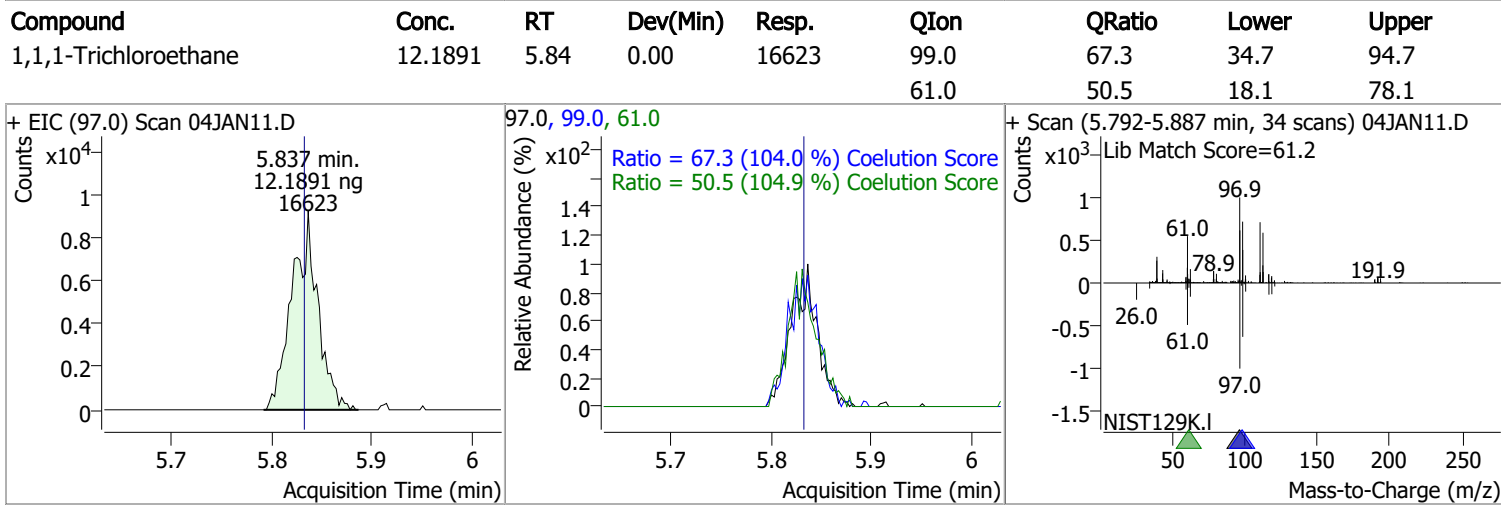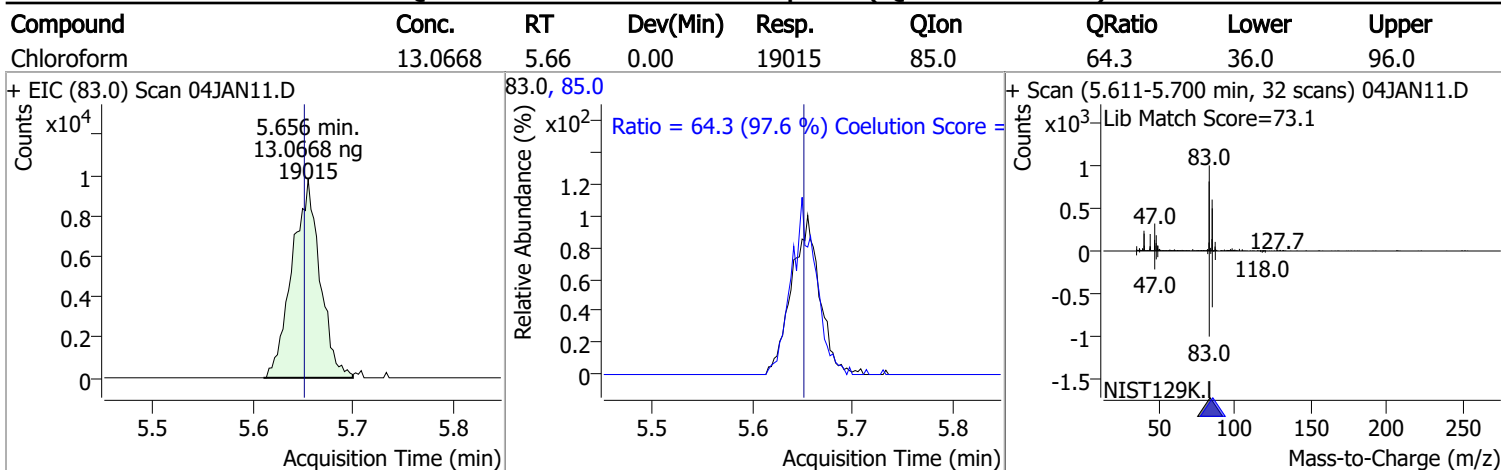




# Quantitation Results Report (QT Reviewed)

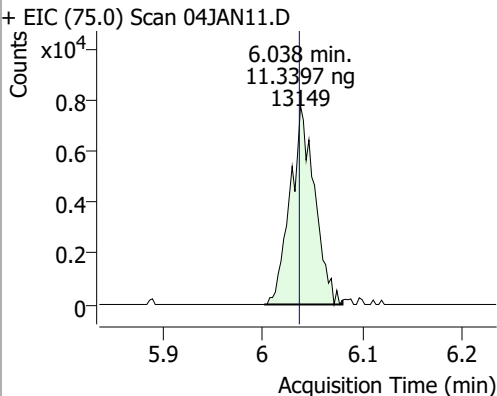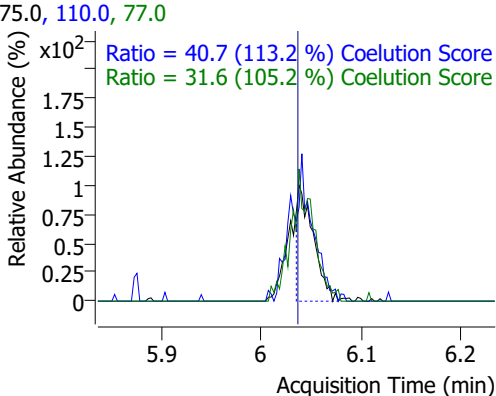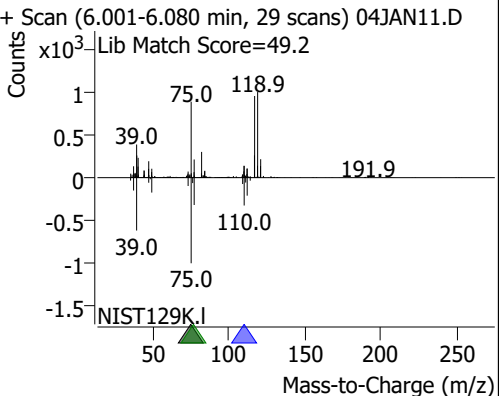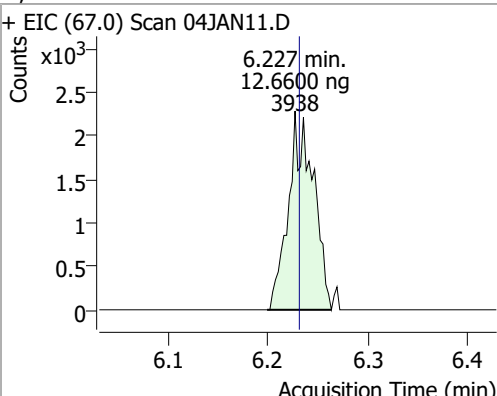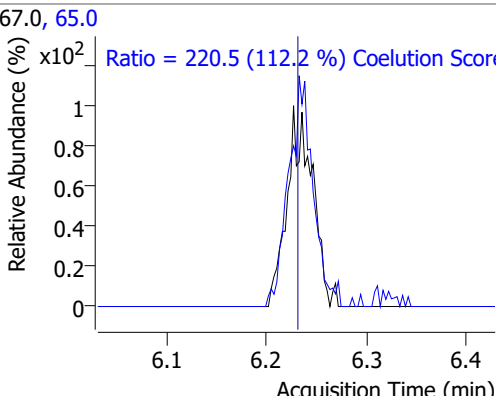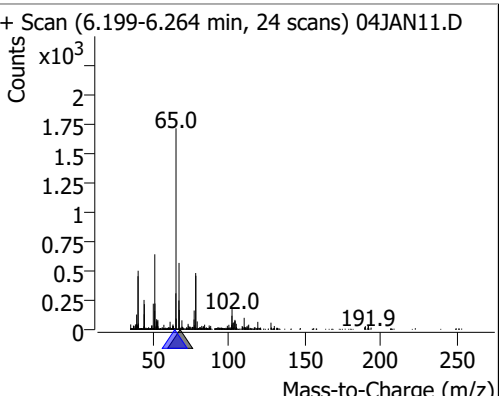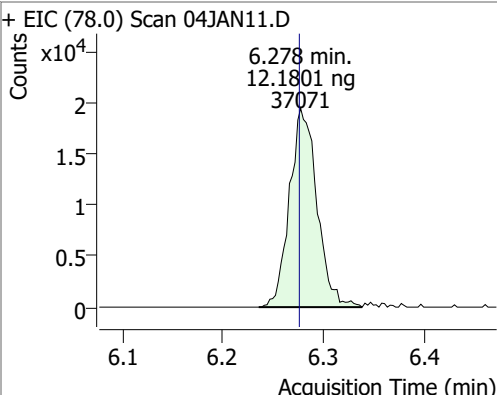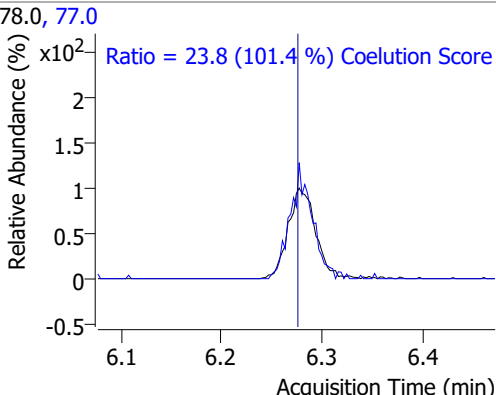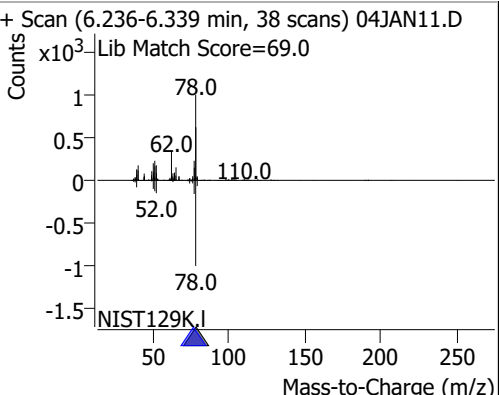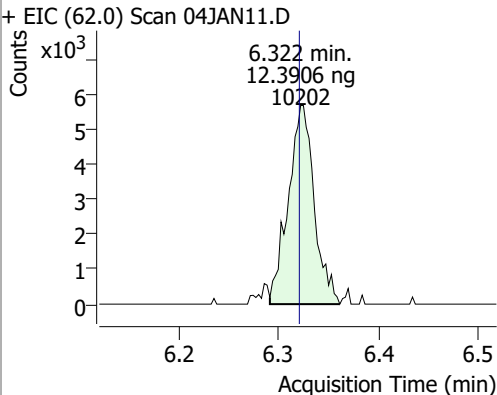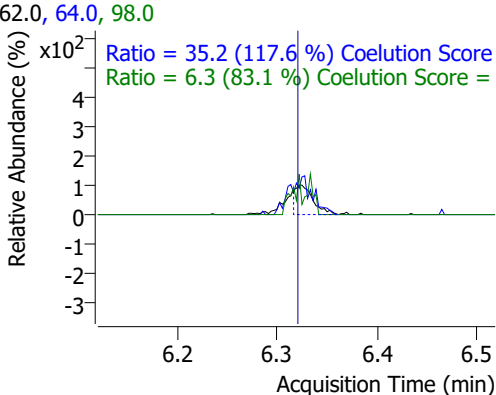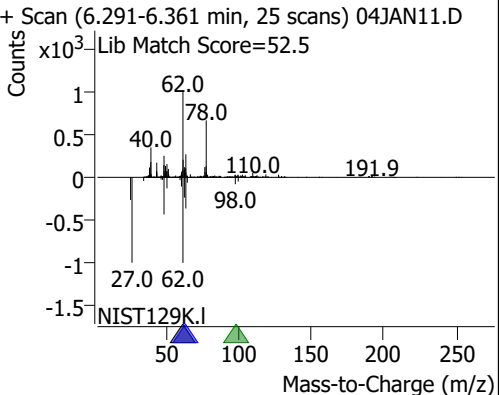
| Compound                                                                           | Conc.                                                                                | RT   | Dev(Min)                                                                              | Resp. | QIon          | QRatio                                       | Lower      | Upper        |
|------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------|------|---------------------------------------------------------------------------------------|-------|---------------|----------------------------------------------|------------|--------------|
| 1,1-Dichloropropene                                                                | 11.3397                                                                              | 6.04 | 0.00                                                                                  | 13149 | 110.0<br>77.0 | 40.7<br>31.6                                 | 5.9<br>0.1 | 65.9<br>60.1 |
| + EIC (75.0) Scan 04JAN11.D                                                        |                                                                                      |      | 75.0, 110.0, 77.0                                                                     |       |               | + Scan (6.001-6.080 min, 29 scans) 04JAN11.D |            |              |
|    |    |      |    |       |               |                                              |            |              |
| 1,2-Dichloroethane-d4                                                              | 12.6600                                                                              | 6.23 | -0.01                                                                                 | 3938  | 65.0          | 220.5                                        | 166.5      | 226.5        |
| + EIC (67.0) Scan 04JAN11.D                                                        |                                                                                      |      | 67.0, 65.0                                                                            |       |               | + Scan (6.199-6.264 min, 24 scans) 04JAN11.D |            |              |
|   |   |      |   |       |               |                                              |            |              |
| Benzene                                                                            | 12.1801                                                                              | 6.28 | 0.00                                                                                  | 37071 | 77.0          | 23.8                                         | 0.0        | 53.5         |
| + EIC (78.0) Scan 04JAN11.D                                                        |                                                                                      |      | 78.0, 77.0                                                                            |       |               | + Scan (6.236-6.339 min, 38 scans) 04JAN11.D |            |              |
|  |  |      |  |       |               |                                              |            |              |
| 1,2-Dichloroethane                                                                 | 12.3906                                                                              | 6.32 | 0.00                                                                                  | 10202 | 64.0<br>98.0  | 35.2<br>6.3                                  | 0.0<br>0.0 | 59.9<br>37.6 |
| + EIC (62.0) Scan 04JAN11.D                                                        |                                                                                      |      | 62.0, 64.0, 98.0                                                                      |       |               | + Scan (6.291-6.361 min, 25 scans) 04JAN11.D |            |              |
|  |  |      |  |       |               |                                              |            |              |

# Quantitation Results Report (QT Reviewed)


| Compound        | Conc.   | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|-----------------|---------|------|----------|-------|-------|--------|-------|-------|
| Trichloroethene | 11.6753 | 7.02 | -0.01    | 10442 | 130.0 | 109.7  | 71.5  | 131.5 |
|                 |         |      |          |       | 97.0  | 66.1   | 34.1  | 94.1  |



| Compound            | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|---------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloropropane | 12.0602 | 7.27 | 0.00     | 9488  | 76.0 | 38.8   | 8.2   | 68.2  |




| Compound       | Conc.   | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|----------------|---------|------|----------|-------|-------|--------|-------|-------|
| Dibromomethane | 14.0619 | 7.40 | 0.00     | 4675  | 173.5 | 106.3  | 83.7  | 143.7 |
|                |         |      |          |       | 95.0  | 75.0   | 52.2  | 112.2 |

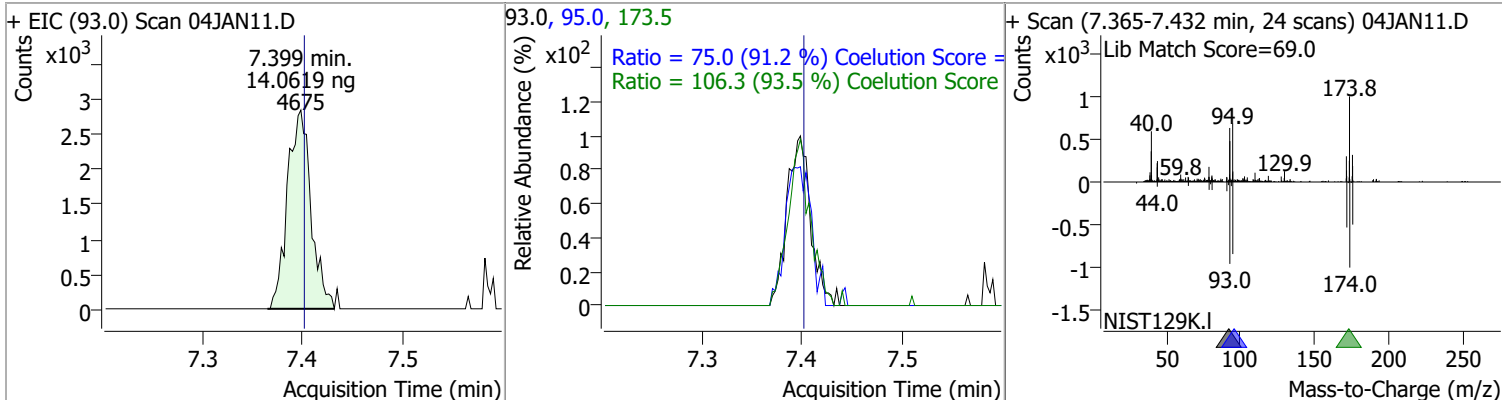


# Quantitation Results Report (QT Reviewed)


| Compound             | Conc.   | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|----------------------|---------|------|----------|-------|-------|--------|-------|-------|
| Bromodichloromethane | 12.6014 | 7.59 | 0.00     | 11562 | 85.0  | 62.3   | 34.5  | 94.5  |
|                      |         |      |          |       | 127.0 | 8.2    | 0.0   | 39.6  |

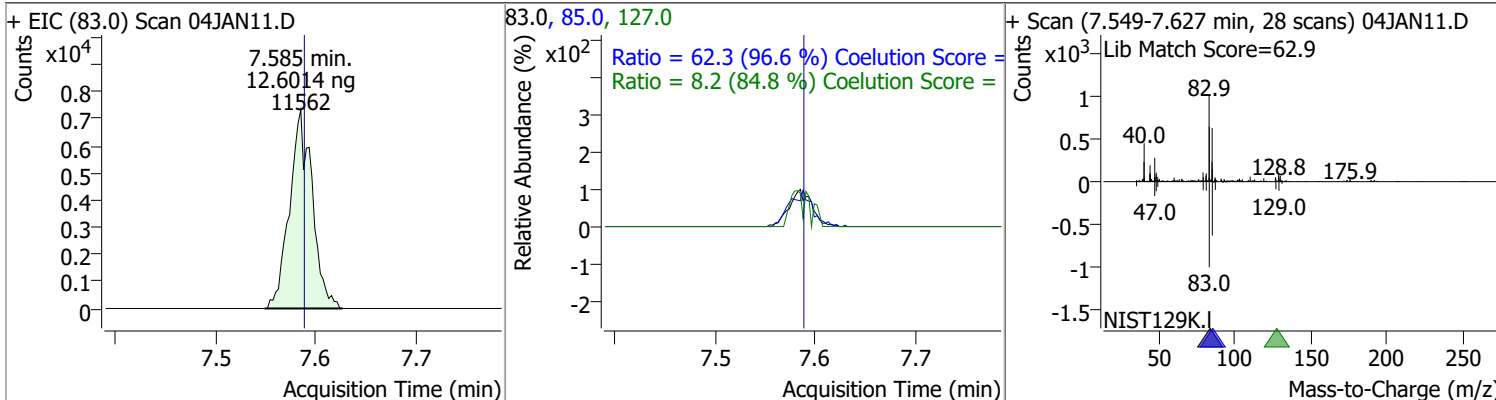










| Compound                | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------------|---------|------|----------|-------|------|--------|-------|-------|
| cis-1,3-Dichloropropene | 12.0738 | 8.06 | 0.00     | 12525 | 39.0 | 57.8   | 23.3  | 83.3  |
|                         |         |      |          |       | 77.0 | 28.1   | 1.0   | 61.0  |

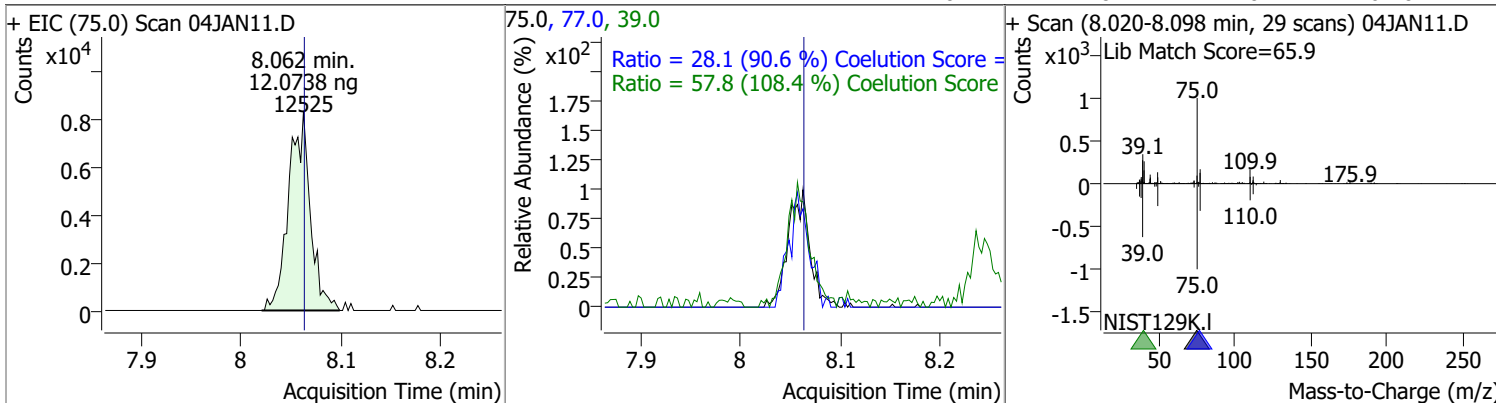













| Compound   | Conc.   | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|------------|---------|------|----------|-------|-------|--------|-------|-------|
| Toluene-d8 | 11.3089 | 8.32 | 0.00     | 32318 | 100.0 | 63.3   | 34.4  | 94.4  |
|            |         |      |          |       | 99.0  | 8.9    | 0.0   | 39.6  |

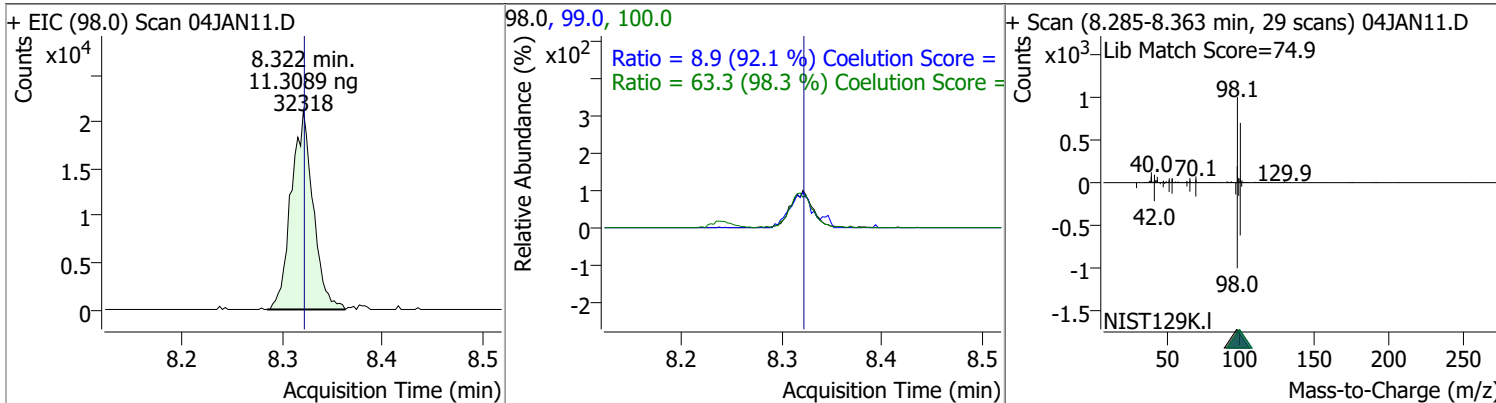





# Quantitation Results Report (QT Reviewed)

| Compound                                                                           | Conc.                                                                                | RT   | Dev(Min)                                                                              | Resp.    | QIon | QRatio                                       | Lower | Upper |
|------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------|------|---------------------------------------------------------------------------------------|----------|------|----------------------------------------------|-------|-------|
| Toluene                                                                            | 11.2899                                                                              | 8.39 | 0.00                                                                                  | 21794    | 91.0 | 172.2                                        | 145.8 | 205.8 |
| + EIC (92.0) Scan 04JAN11.D                                                        |                                                                                      |      | 92.0, 91.0                                                                            |          |      | + Scan (8.349-8.419 min, 25 scans) 04JAN11.D |       |       |
|    |    |      |    |          |      |                                              |       |       |
|                                                                                    |                                                                                      |      |                                                                                       |          |      | Ratio = 172.2 (98.0 %) Coelution Score       |       |       |
| trans-1,3-Dichloropropene                                                          | 11.7589                                                                              | 8.65 | 0.01                                                                                  | 8683     | 39.0 | 53.4                                         | 23.4  | 83.4  |
|                                                                                    |                                                                                      |      |                                                                                       |          | 77.0 | 35.5                                         | 2.4   | 62.4  |
| + EIC (75.0) Scan 04JAN11.D                                                        |                                                                                      |      | 75.0, 77.0, 39.0                                                                      |          |      | + Scan (8.603-8.676 min, 27 scans) 04JAN11.D |       |       |
|   |   |      |   |          |      |                                              |       |       |
|                                                                                    |                                                                                      |      |                                                                                       |          |      | Ratio = 35.5 (109.6 %) Coelution Score       |       |       |
|                                                                                    |                                                                                      |      |                                                                                       |          |      | Ratio = 53.4 (100.1 %) Coelution Score       |       |       |
| 1,1,2-Trichloroethane                                                              | 13.2340                                                                              | 8.82 | 0.01                                                                                  | 5090 (m) | 97.0 | 105.6                                        | 84.6  | 144.6 |
|                                                                                    |                                                                                      |      |                                                                                       |          | 85.0 | 59.6                                         | 37.6  | 97.6  |
| + EIC (83.0) Scan 04JAN11.D                                                        |                                                                                      |      | 83.0, 97.0, 85.0                                                                      |          |      | + Scan (8.768-8.882 min, 41 scans) 04JAN11.D |       |       |
|  |  |      |  |          |      |                                              |       |       |
|                                                                                    |                                                                                      |      |                                                                                       |          |      | Ratio = 105.6 (92.1 %) Coelution Score       |       |       |
|                                                                                    |                                                                                      |      |                                                                                       |          |      | Ratio = 59.6 (88.1 %) Coelution Score        |       |       |

# Quantitation Results Report (QT Reviewed)

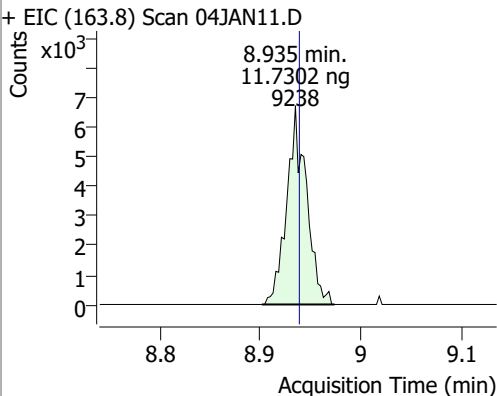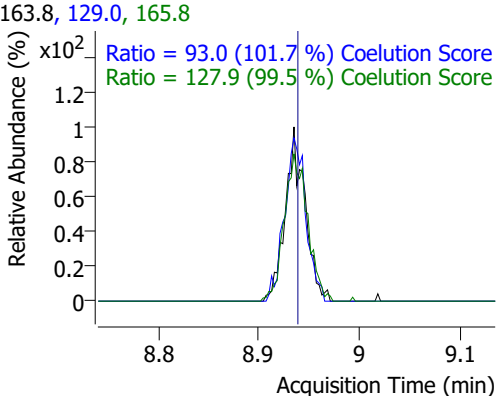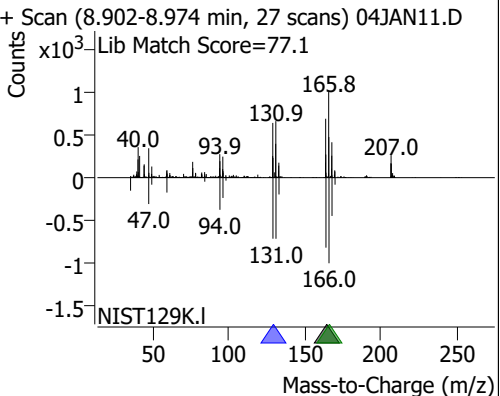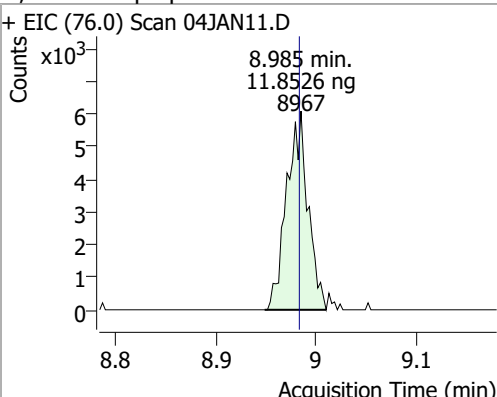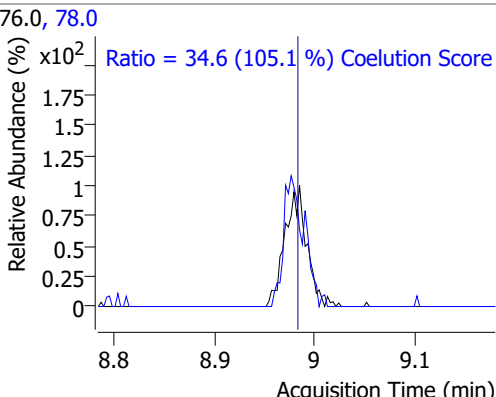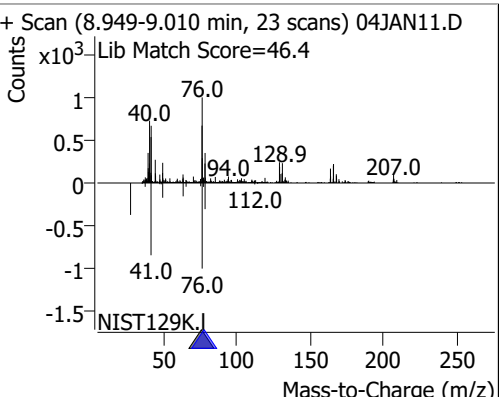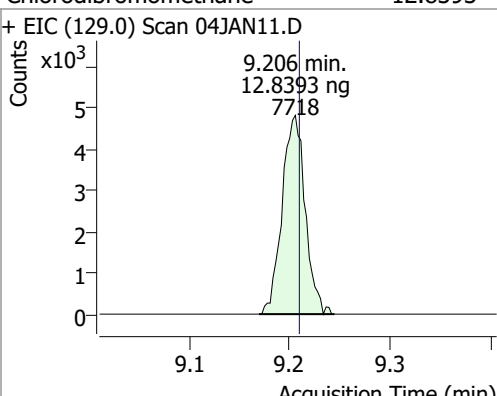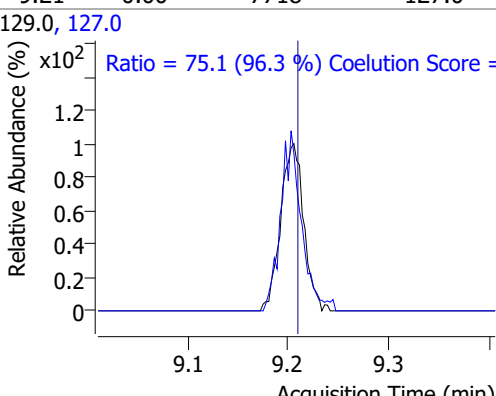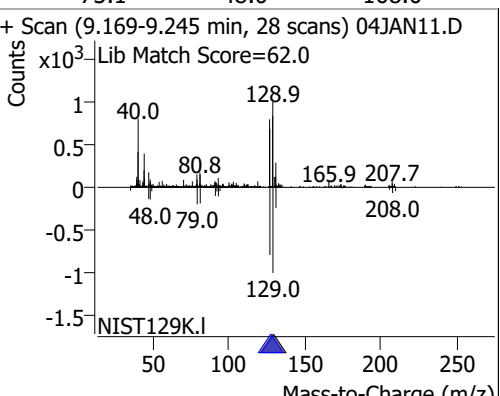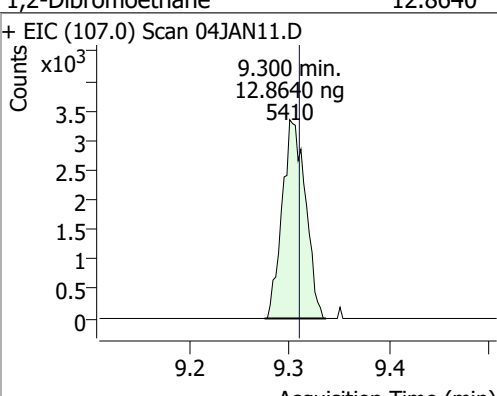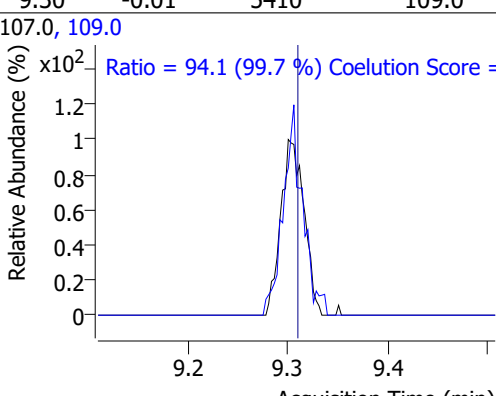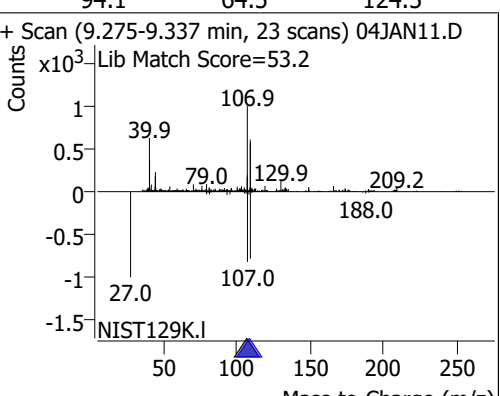
| Compound                                                                           | Conc.                                                                                | RT   | Dev(Min)                                                                              | Resp. | QIon           | QRatio                                       | Lower        | Upper          |
|------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------|------|---------------------------------------------------------------------------------------|-------|----------------|----------------------------------------------|--------------|----------------|
| Tetrachloroethene                                                                  | 11.7302                                                                              | 8.94 | 0.00                                                                                  | 9238  | 165.8<br>129.0 | 127.9<br>93.0                                | 98.6<br>61.5 | 158.6<br>121.5 |
| + EIC (163.8) Scan 04JAN11.D                                                       |                                                                                      |      | 163.8, 129.0, 165.8                                                                   |       |                | + Scan (8.902-8.974 min, 27 scans) 04JAN11.D |              |                |
|    |    |      |    |       |                |                                              |              |                |
| Ratio = 93.0 (101.7 %) Coelution Score                                             |                                                                                      |      | Ratio = 127.9 (99.5 %) Coelution Score                                                |       |                |                                              |              |                |
| 1,3-Dichloropropane                                                                | 11.8526                                                                              | 8.99 | 0.01                                                                                  | 8967  | 78.0           | 34.6                                         | 2.9          | 62.9           |
| + EIC (76.0) Scan 04JAN11.D                                                        |                                                                                      |      | 76.0, 78.0                                                                            |       |                | + Scan (8.949-9.010 min, 23 scans) 04JAN11.D |              |                |
|   |   |      |   |       |                |                                              |              |                |
| Ratio = 34.6 (105.1 %) Coelution Score                                             |                                                                                      |      |                                                                                       |       |                |                                              |              |                |
| Chlorodibromomethane                                                               | 12.8393                                                                              | 9.21 | 0.00                                                                                  | 7718  | 127.0          | 75.1                                         | 48.0         | 108.0          |
| + EIC (129.0) Scan 04JAN11.D                                                       |                                                                                      |      | 129.0, 127.0                                                                          |       |                | + Scan (9.169-9.245 min, 28 scans) 04JAN11.D |              |                |
|  |  |      |  |       |                |                                              |              |                |
| Ratio = 75.1 (96.3 %) Coelution Score                                              |                                                                                      |      |                                                                                       |       |                |                                              |              |                |
| 1,2-Dibromoethane                                                                  | 12.8640                                                                              | 9.30 | -0.01                                                                                 | 5410  | 109.0          | 94.1                                         | 64.5         | 124.5          |
| + EIC (107.0) Scan 04JAN11.D                                                       |                                                                                      |      | 107.0, 109.0                                                                          |       |                | + Scan (9.275-9.337 min, 23 scans) 04JAN11.D |              |                |
|  |  |      |  |       |                |                                              |              |                |
| Ratio = 94.1 (99.7 %) Coelution Score                                              |                                                                                      |      |                                                                                       |       |                |                                              |              |                |

# Quantitation Results Report (QT Reviewed)

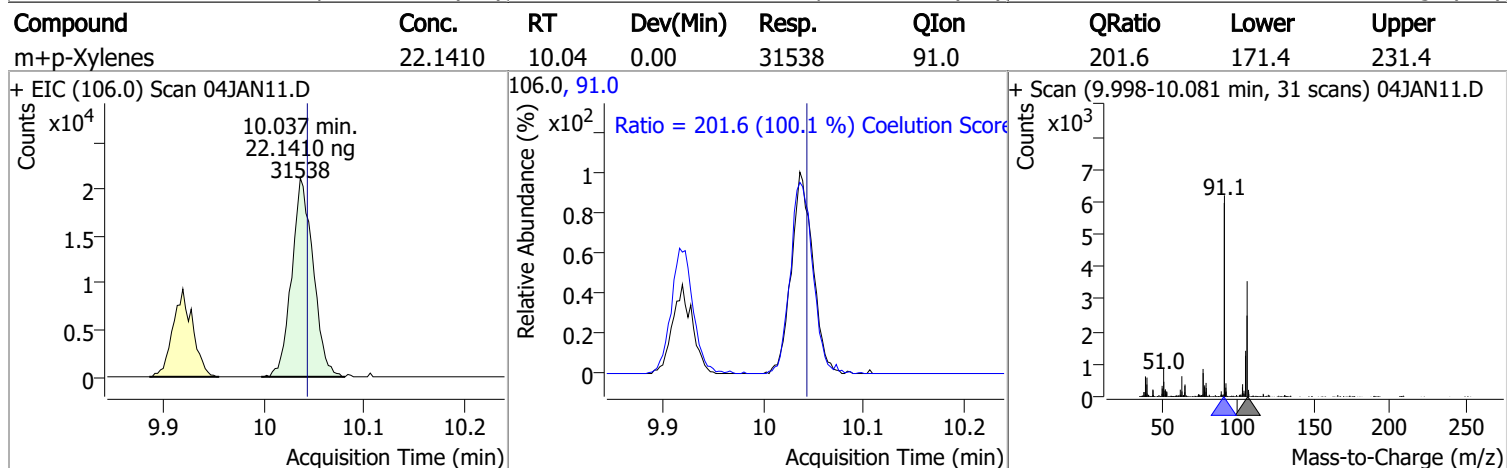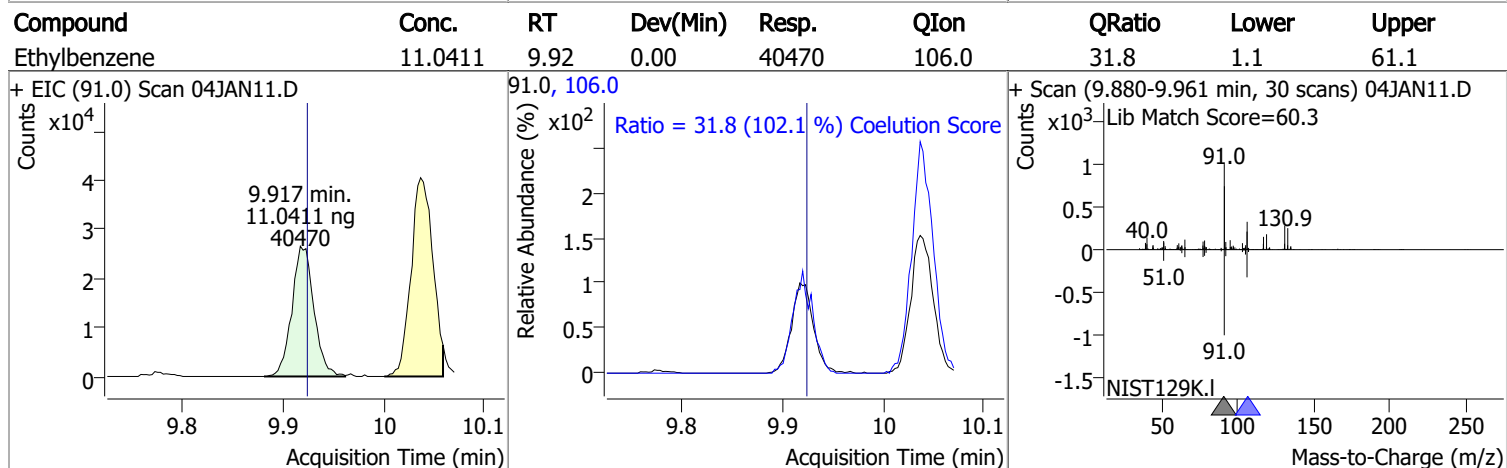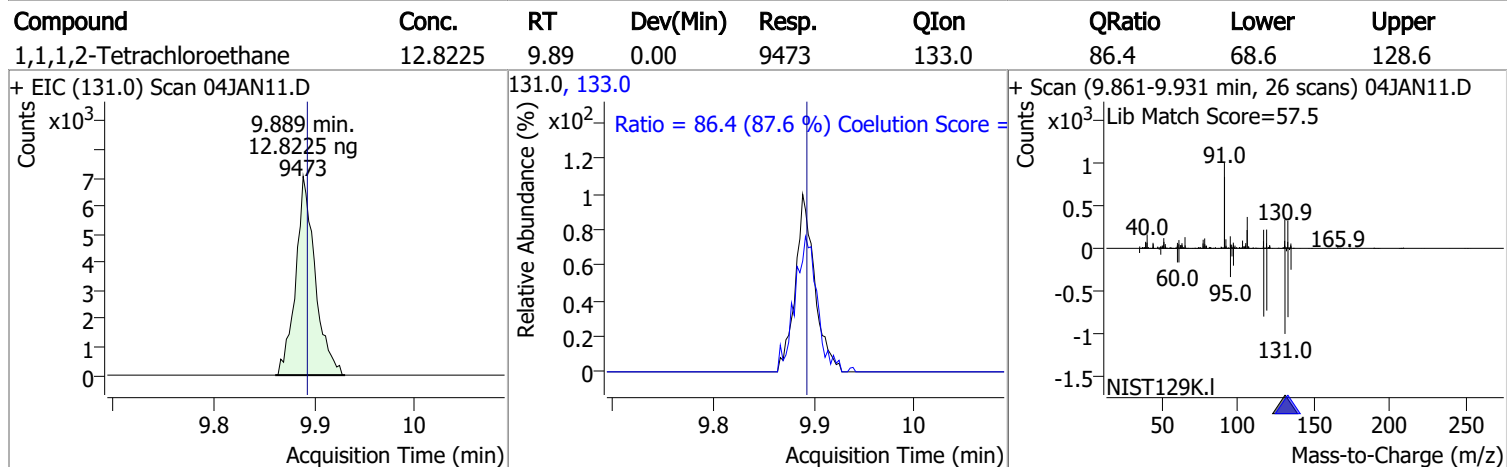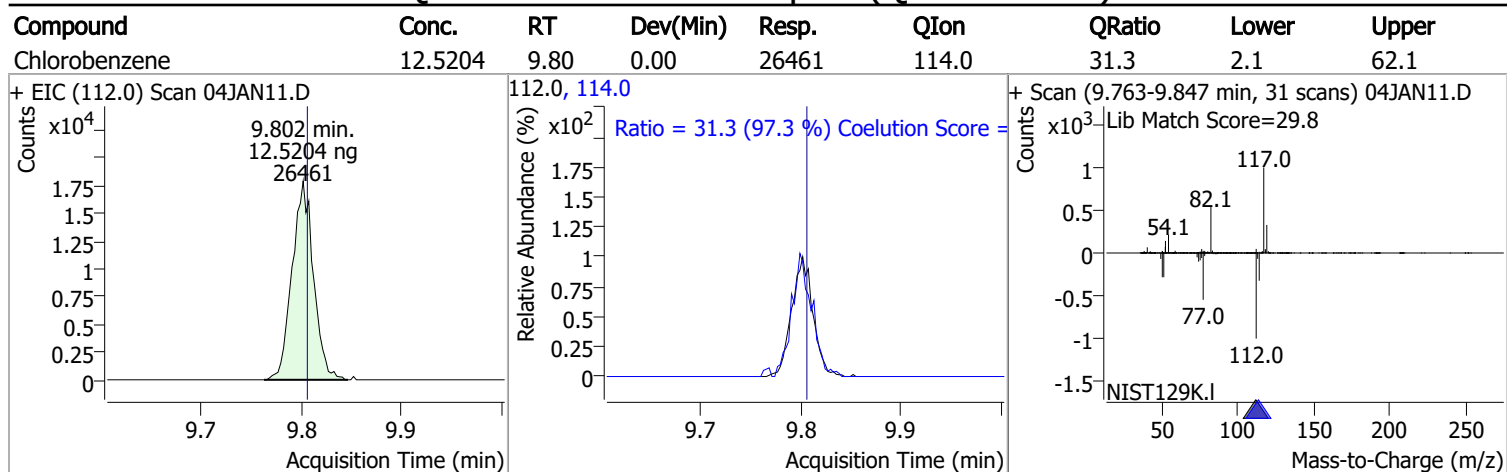


# Quantitation Results Report (QT Reviewed)


| Compound | Conc.   | RT    | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|---------|-------|----------|-------|------|--------|-------|-------|
| o-Xylene | 10.6612 | 10.43 | 0.00     | 13519 | 91.0 | 225.2  | 183.1 | 243.1 |




| Compound | Conc.   | RT    | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|---------|-------|----------|-------|------|--------|-------|-------|
| Styrene  | 11.4968 | 10.45 | 0.00     | 23472 | 78.0 | 49.5   | 19.6  | 79.6  |



| Compound  | Conc.   | RT    | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|-----------|---------|-------|----------|-------|-------|--------|-------|-------|
| Bromoform | 11.7860 | 10.62 | 0.00     | 3652  | 170.5 | 55.5   | 22.1  | 82.1  |
|           |         |       |          |       | 174.5 | 58.2   | 20.1  | 80.1  |




| Compound             | Conc.   | RT    | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|----------------------|---------|-------|----------|-------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 11.3393 | 10.95 | -0.01    | 10059 | 174.0 | 98.3   | 61.7  | 121.7 |
|                      |         |       |          |       | 176.0 | 96.5   | 60.6  | 120.6 |




# Quantitation Results Report (QT Reviewed)


| Compound     | Conc.   | RT    | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|--------------|---------|-------|----------|-------|-------|--------|-------|-------|
| Bromobenzene | 12.3310 | 11.10 | 0.00     | 9663  | 77.0  | 140.9  | 115.7 | 175.7 |
|              |         |       |          |       | 158.0 | 101.5  | 66.5  | 126.5 |

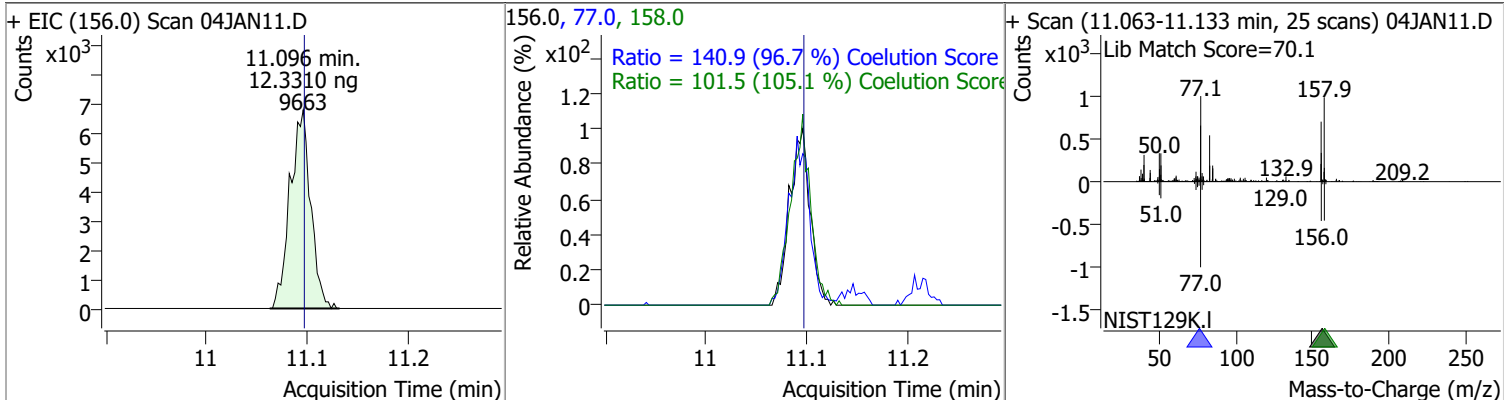


| Compound                  | Conc.   | RT    | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|---------|-------|----------|-------|------|--------|-------|-------|
| 1,1,2,2-Tetrachloroethane | 12.8437 | 11.12 | 0.00     | 5793  | 85.0 | 67.4   | 36.2  | 96.2  |

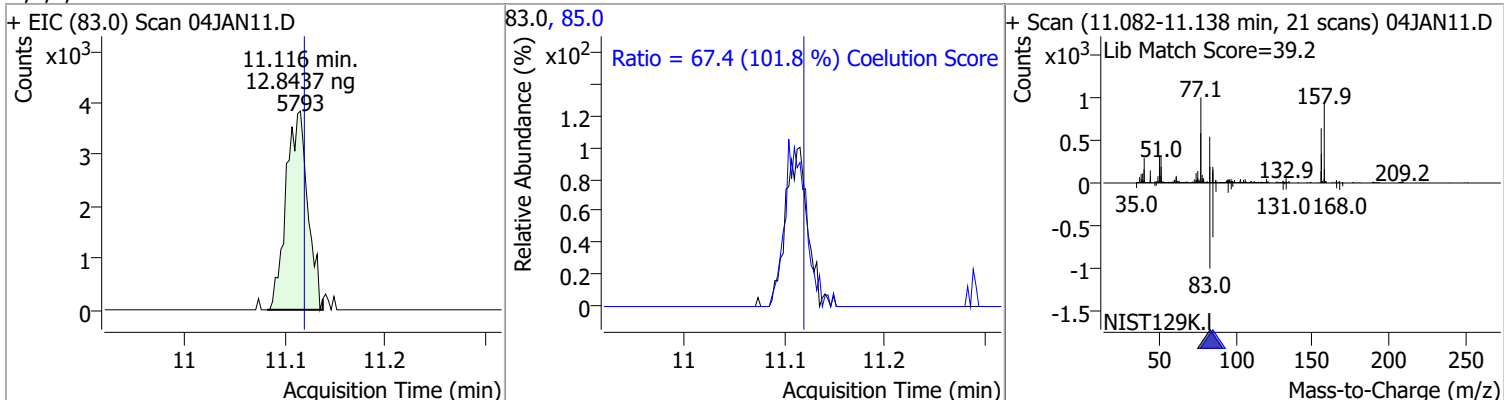

| Compound               | Conc.   | RT    | Dev(Min) | Resp.    | QIon  | QRatio | Lower | Upper |
|------------------------|---------|-------|----------|----------|-------|--------|-------|-------|
| 1,2,3-Trichloropropane | 13.7084 | 11.14 | 0.00     | 1654 (m) | 112.0 | 64.0   | 33.5  | 93.5  |

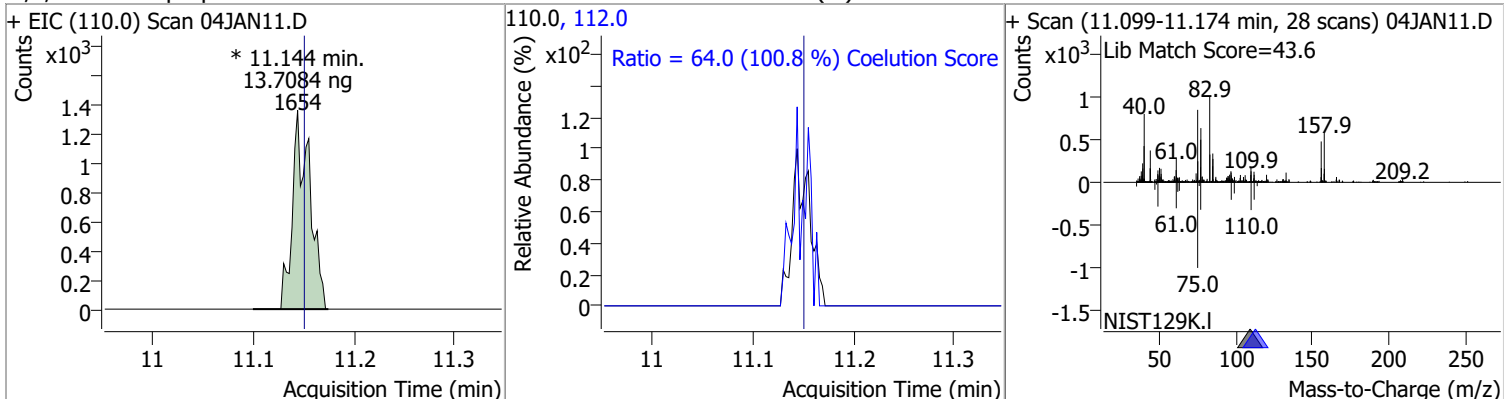

| Compound        | Conc.   | RT    | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|---------|-------|----------|-------|------|--------|-------|-------|
| 2-Chlorotoluene | 11.1977 | 11.29 | 0.00     | 8731  | 91.0 | 293.4  | 252.3 | 312.3 |

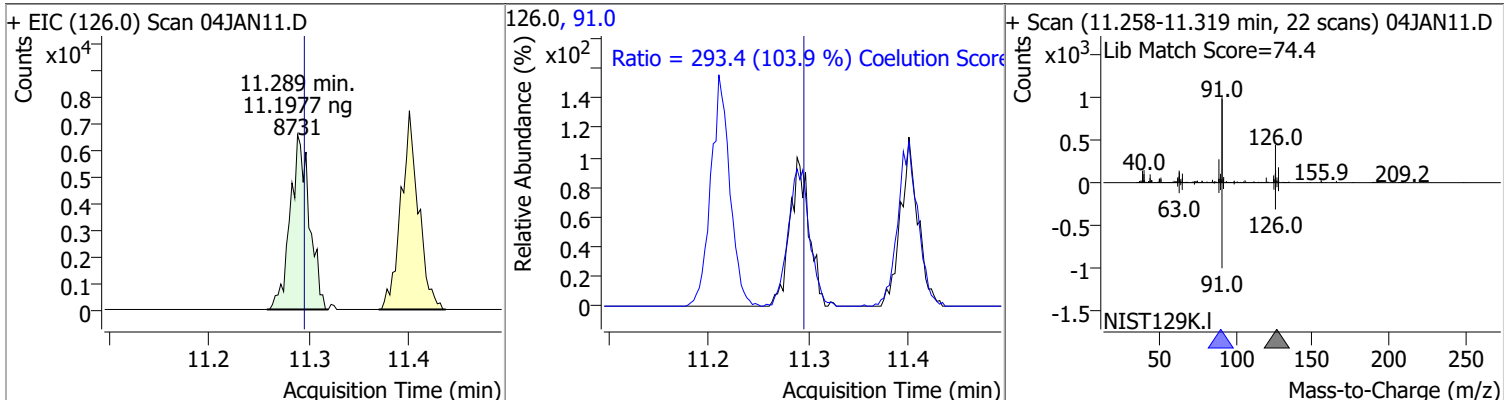






# Quantitation Results Report (QT Reviewed)

| Compound                     | Conc.   | RT    | Dev(Min)            | Resp. | QIon  | QRatio                                         | Lower | Upper |
|------------------------------|---------|-------|---------------------|-------|-------|------------------------------------------------|-------|-------|
| 4-Chlorotoluene              | 11.2233 | 11.40 | 0.00                | 28532 | 126.0 | 31.7                                           | 1.7   | 61.7  |
| + EIC (91.0) Scan 04JAN11.D  |         |       | 91.0, 126.0         |       |       | + Scan (11.364-11.439 min, 28 scans) 04JAN11.D |       |       |
|                              |         |       |                     |       |       |                                                |       |       |
| 1,3-Dichlorobenzene          | 11.8473 | 12.04 | 0.01                | 16932 | 148.0 | 64.2                                           | 33.6  | 93.6  |
| + EIC (146.0) Scan 04JAN11.D |         |       | 146.0, 111.0, 148.0 |       |       | + Scan (12.000-12.067 min, 25 scans) 04JAN11.D |       |       |
|                              |         |       |                     |       |       |                                                |       |       |
| 1,4-Dichlorobenzene          | 11.9662 | 12.12 | 0.00                | 17438 | 148.0 | 70.5                                           | 33.1  | 93.1  |
| + EIC (146.0) Scan 04JAN11.D |         |       | 146.0, 111.0, 148.0 |       |       | + Scan (12.089-12.159 min, 25 scans) 04JAN11.D |       |       |
|                              |         |       |                     |       |       |                                                |       |       |


# Quantitation Results Report (QT Reviewed)

| Compound            | Conc.   | RT    | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|---------------------|---------|-------|----------|-------|-------|--------|-------|-------|
| 1,2-Dichlorobenzene | 12.1423 | 12.49 | 0.00     | 14666 | 148.0 | 66.1   | 33.9  | 93.9  |
|                     |         |       |          |       | 111.0 | 40.3   | 11.0  | 71.0  |



# Quantitation Results Report (QT Reviewed)

|                |                                     |                   |                       |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File      | 04JAN12.D                           | Operator          | MSC                   |
| Acq. Method    | 5975CACQF.M                         | Acq. Date-Time    | 1/4/2022 4:28:05 PM   |
| Sample Name    | ICAL010422_3                        | Instrument        | VOA5975C              |
| Vial           | 12                                  | Multiplier        | 1.00                  |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m  | Comment           |                       |
| Tune File      | BFB_Atune3.u                        | Tune Date         | 10/11/2021 4:02:00 PM |
| Batch Name     | VG010422_8260B.batch.bin            | Last Calib Update | 1/9/2022 8:59:52 PM   |
| Ref Library    | \\MASSHUNTER\Org\Library\NIST129K.I |                   |                       |

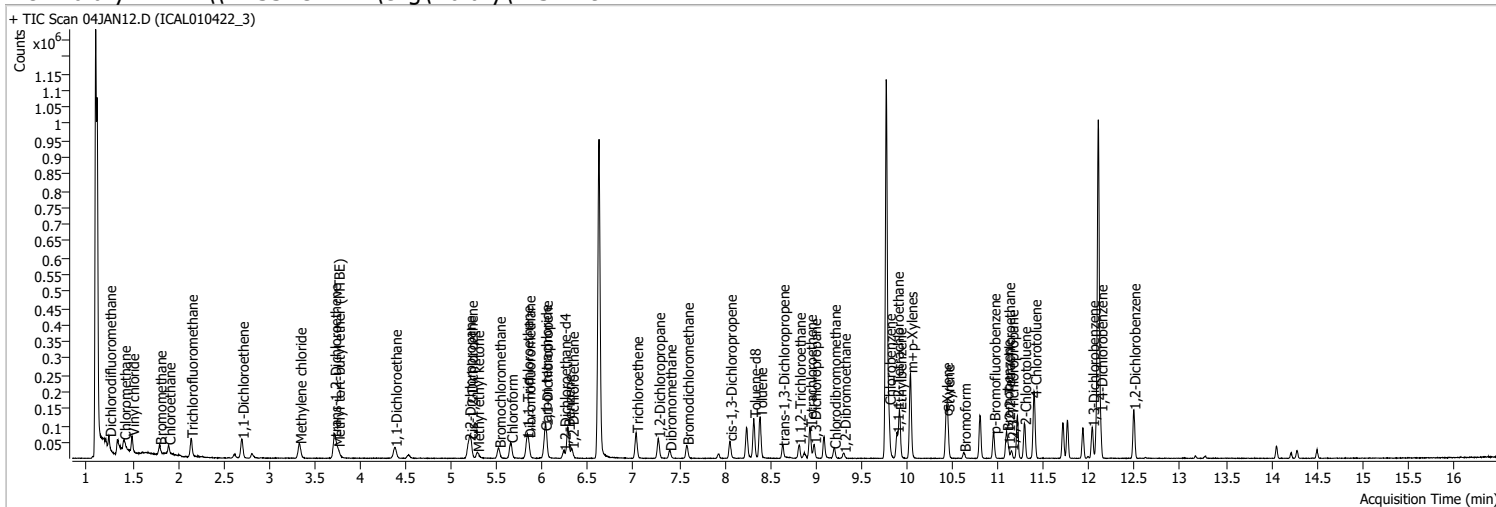













| Compound                           | RT                   | QIon  | Resp.  | Conc.             | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|-------------------|-------|----------|
| <b>Internal Standards</b>          |                      |       |        |                   |       |          |
| M Fluorobenzene                    | 6.621                | 96.0  | 791270 | 250.0000          | ng    | -0.003   |
| M Chlorobenzene-d5                 | 9.775                | 82.0  | 301338 | 250.0000          | ng    | 0.003    |
| M 1,4-Dichlorobenzene-d4           | 12.103               | 152.0 | 240335 | 250.0000          | ng    | 0.003    |
| <b>System Monitoring Compounds</b> |                      |       |        |                   |       |          |
| S Dibromofluoromethane             | 5.845                | 113.0 | 19100  | 25.6219           | ng    | 0.000    |
| Spiked Amount: 250.000             | Range: 80.0 - 119.0% |       |        | Recovery = 10.25% | *     |          |
| S 1,2-Dichloroethane-d4            | 6.236                | 67.0  | 8284   | 25.7280           | ng    | 0.003    |
| Spiked Amount: 250.000             | Range: 81.0 - 118.0% |       |        | Recovery = 10.29% | *     |          |
| S Toluene-d8                       | 8.319                | 98.0  | 67673  | 23.3046           | ng    | 0.000    |
| Spiked Amount: 250.000             | Range: 89.0 - 112.0% |       |        | Recovery = 9.32%  | *     |          |
| S p-Bromofluorobenzene             | 10.951               | 95.0  | 22267  | 25.2899           | ng    | -0.003   |
| Spiked Amount: 250.000             | Range: 85.0 - 114.0% |       |        | Recovery = 10.12% | *     |          |
| <b>Target Compounds</b>            |                      |       |        |                   |       |          |
| T Dichlorodifluoromethane          | 1.244                | 85.0  | 26627  | 25.6793           | ng    | 99       |
| T Chloromethane                    | 1.406                | 50.0  | 33153  | 26.3422           | ng    | 95       |
| T Vinyl chloride                   | 1.495                | 62.0  | 29046  | 25.6488           | ng    | 80       |
| T Bromomethane                     | 1.796                | 96.0  | 13054  | 25.7793           | ng    | 99       |
| T Chloroethane                     | 1.897                | 64.0  | 14646  | 26.1250           | ng    | m 92     |
| T Trichlorofluoromethane           | 2.142                | 101.0 | 37464  | 26.6531           | ng    | 98       |
| T 1,1-Dichloroethene               | 2.700                | 96.0  | 20631  | 25.8849           | ng    | 93       |
| T Methylene chloride               | 3.333                | 49.0  | 30908  | 26.3058           | ng    | 100      |
| T trans-1,2-Dichloroethene         | 3.712                | 96.0  | 20706  | 25.4641           | ng    | 97       |
| T Methyl tert-butyl ether (MTBE)   | 3.754                | 73.0  | 24218  | 23.0418           | ng    | 92       |
| T 1,1-Dichloroethane               | 4.379                | 63.0  | 38874  | 25.6835           | ng    | 97       |
| T 2,2-Dichloropropane              | 5.190                | 77.0  | 29793  | 26.2692           | ng    | 100      |
| T cis-1,2-Dichloroethene           | 5.212                | 96.0  | 20252  | 24.5653           | ng    | 98       |
| T Methyl ethyl ketone              | 5.282                | 43.0  | 26248  | 235.0504          | ng    | 98       |
| T Bromochloromethane               | 5.522                | 128.0 | 8688   | 25.4383           | ng    | 98       |
| T Chloroform                       | 5.653                | 83.0  | 36413  | 24.1734           | ng    | 97       |

# Quantitation Results Report (QT Reviewed)

| Compound                    | RT     | QIon  | Resp. | Conc.   | Units | Dev(Min) |
|-----------------------------|--------|-------|-------|---------|-------|----------|
| T 1,1,1-Trichloroethane     | 5.826  | 97.0  | 35547 | 25.1809 | ng    | 96       |
| T Carbon tetrachloride      | 6.024  | 117.0 | 34462 | 24.7773 | ng    | 99       |
| T 1,1-Dichloropropene       | 6.038  | 75.0  | 29241 | 24.3617 | ng    | 96       |
| T Benzene                   | 6.278  | 78.0  | 74956 | 23.7919 | ng    | 97       |
| T 1,2-Dichloroethane        | 6.322  | 62.0  | 19996 | 23.4616 | ng    | 97       |
| T Trichloroethene           | 7.028  | 95.0  | 21946 | 24.1484 | ng    | 98       |
| T 1,2-Dichloropropane       | 7.270  | 63.0  | 20077 | 25.1147 | ng    | 98       |
| T Dibromomethane            | 7.393  | 93.0  | 8055  | 23.8439 | ng    | 97       |
| T Bromodichloromethane      | 7.583  | 83.0  | 22743 | 24.3940 | ng    | 98       |
| T cis-1,3-Dichloropropene   | 8.057  | 75.0  | 24511 | 23.2528 | ng    | 97       |
| T Toluene                   | 8.389  | 92.0  | 46355 | 23.6319 | ng    | 99       |
| T trans-1,3-Dichloropropene | 8.634  | 75.0  | 17850 | 23.7894 | ng    | 97       |
| T 1,1,2-Trichloroethane     | 8.815  | 83.0  | 10099 | 25.8400 | ng    | 95       |
| T Tetrachloroethene         | 8.935  | 163.8 | 20322 | 25.3948 | ng    | 97       |
| T 1,3-Dichloropropane       | 8.983  | 76.0  | 18745 | 24.3839 | ng    | 99       |
| T Chlorodibromomethane      | 9.197  | 129.0 | 14873 | 24.3492 | ng    | 99       |
| T 1,2-Dibromoethane         | 9.309  | 107.0 | 10410 | 24.3601 | ng    | 95       |
| T Chlorobenzene             | 9.802  | 112.0 | 53047 | 24.7015 | ng    | 100      |
| T 1,1,1,2-Tetrachloroethane | 9.889  | 131.0 | 18130 | 24.1509 | ng    | 100      |
| T Ethylbenzene              | 9.917  | 91.0  | 88428 | 23.7421 | ng    | 100      |
| T m+p-Xylenes               | 10.039 | 106.0 | 66267 | 45.7836 | ng    | 98       |
| T o-Xylene                  | 10.427 | 106.0 | 30463 | 23.6420 | ng    | 98       |
| T Styrene                   | 10.447 | 104.0 | 48569 | 23.4119 | ng    | 97       |
| T Bromoform                 | 10.625 | 172.5 | 7972  | 25.9212 | ng    | 96       |
| T Bromobenzene              | 11.094 | 156.0 | 19259 | 24.7613 | ng    | 94       |
| T 1,1,2,2-Tetrachloroethane | 11.110 | 83.0  | 12440 | 27.7883 | ng    | 93       |
| T 1,2,3-Trichloropropane    | 11.149 | 110.0 | 3200  | 26.7144 | ng    | m 96     |
| T 2-Chlorotoluene           | 11.286 | 126.0 | 19390 | 25.0550 | ng    | 94       |
| T 4-Chlorotoluene           | 11.400 | 91.0  | 61551 | 24.3936 | ng    | 100      |
| T 1,3-Dichlorobenzene       | 12.033 | 146.0 | 36559 | 25.7725 | ng    | 97       |
| T 1,4-Dichlorobenzene       | 12.125 | 146.0 | 36635 | 25.3284 | ng    | 92       |
| T 1,2-Dichlorobenzene       | 12.488 | 146.0 | 29899 | 24.9402 | ng    | 98       |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (\*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

# Quantitation Results Report (QT Reviewed)

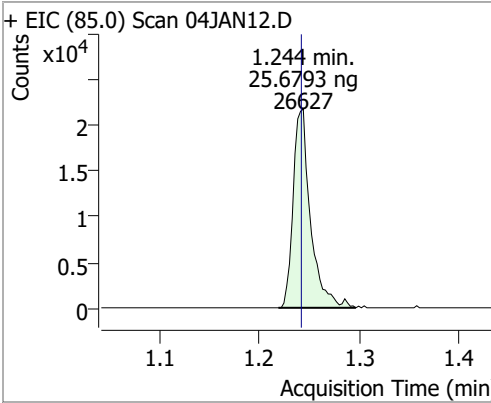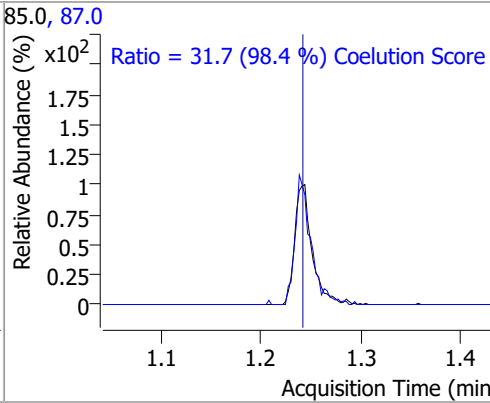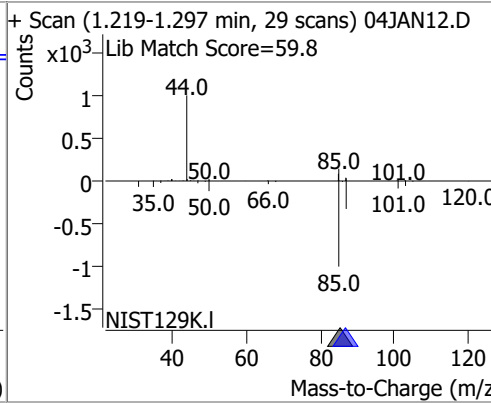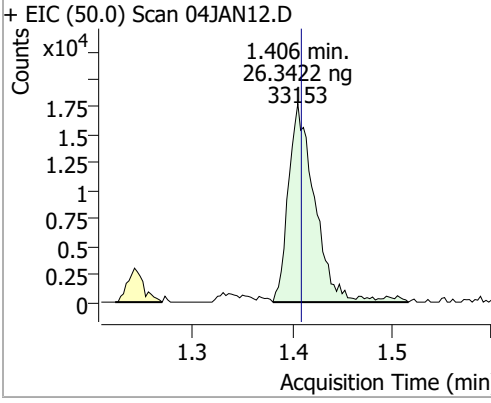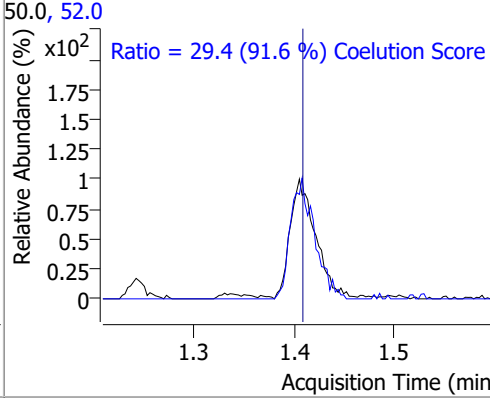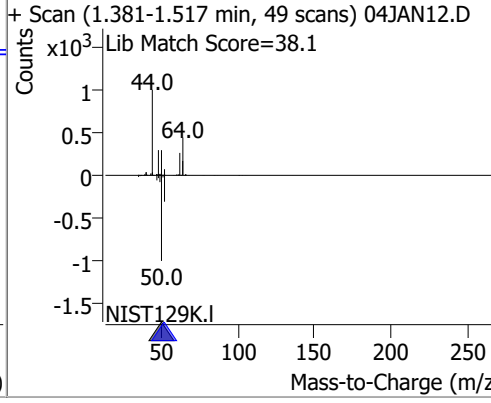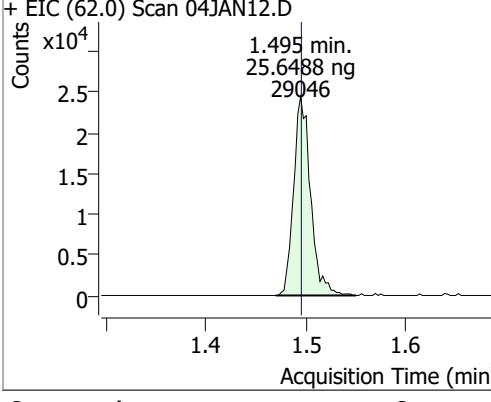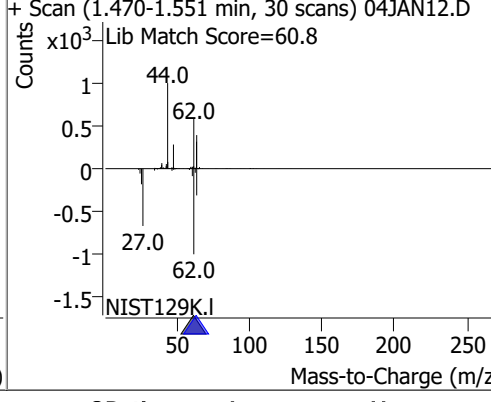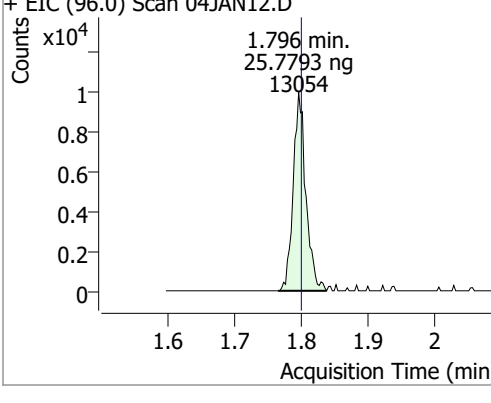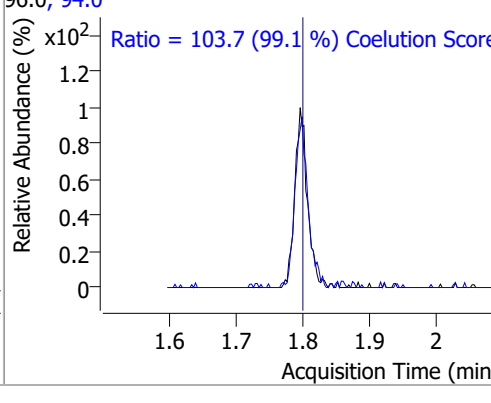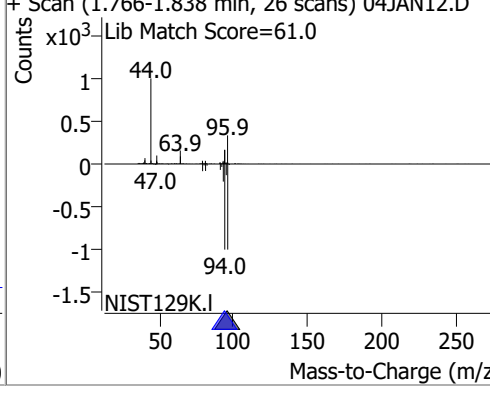
| Compound                                                                                                          | Conc.   | RT   | Dev(Min)                                                                                           | Resp. | QIon | QRatio                                                                                                                                                        | Lower | Upper |
|-------------------------------------------------------------------------------------------------------------------|---------|------|----------------------------------------------------------------------------------------------------|-------|------|---------------------------------------------------------------------------------------------------------------------------------------------------------------|-------|-------|
| Dichlorodifluoromethane                                                                                           | 25.6793 | 1.24 | 0.00                                                                                               | 26627 | 87.0 | 31.7                                                                                                                                                          | 2.3   | 62.3  |
| + EIC (85.0) Scan 04JAN12.D<br>   |         |      | 85.0, 87.0<br>   |       |      | + Scan (1.219-1.297 min, 29 scans) 04JAN12.D<br>Lib Match Score=59.8<br>   |       |       |
| Chloromethane                                                                                                     | 26.3422 | 1.41 | 0.00                                                                                               | 33153 | 52.0 | 29.4                                                                                                                                                          | 2.1   | 62.1  |
| + EIC (50.0) Scan 04JAN12.D<br>  |         |      | 50.0, 52.0<br>  |       |      | + Scan (1.381-1.517 min, 49 scans) 04JAN12.D<br>Lib Match Score=38.1<br>  |       |       |
| Vinyl chloride                                                                                                    | 25.6488 | 1.50 | 0.00                                                                                               | 29046 | 64.0 | 40.6                                                                                                                                                          | 0.0   | 59.9  |
| + EIC (62.0) Scan 04JAN12.D<br> |         |      | 62.0, 64.0<br> |       |      | + Scan (1.470-1.551 min, 30 scans) 04JAN12.D<br>Lib Match Score=60.8<br> |       |       |
| Bromomethane                                                                                                      | 25.7793 | 1.80 | 0.00                                                                                               | 13054 | 94.0 | 103.7                                                                                                                                                         | 74.6  | 134.6 |
| + EIC (96.0) Scan 04JAN12.D<br> |         |      | 96.0, 94.0<br> |       |      | + Scan (1.766-1.838 min, 26 scans) 04JAN12.D<br>Lib Match Score=61.0<br> |       |       |

# Quantitation Results Report (QT Reviewed)


| Compound     | Conc.   | RT   | Dev(Min) | Resp.     | QIon | QRatio | Lower | Upper |
|--------------|---------|------|----------|-----------|------|--------|-------|-------|
| Chloroethane | 26.1250 | 1.90 | 0.00     | 14646 (m) | 66.0 | 34.6   | 0.1   | 60.1  |




| Compound               | Conc.   | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|------------------------|---------|------|----------|-------|-------|--------|-------|-------|
| Trichlorofluoromethane | 26.6531 | 2.14 | 0.00     | 37464 | 103.0 | 62.6   | 34.2  | 94.2  |



| Compound           | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|---------|------|----------|-------|------|--------|-------|-------|
| 1,1-Dichloroethene | 25.8849 | 2.70 | 0.00     | 20631 | 61.0 | 169.5  | 150.3 | 210.3 |
|                    |         |      |          |       | 63.0 | 54.2   | 26.7  | 86.7  |




| Compound           | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|---------|------|----------|-------|------|--------|-------|-------|
| Methylene chloride | 26.3058 | 3.33 | 0.00     | 30908 | 84.0 | 67.0   | 36.9  | 96.9  |
|                    |         |      |          |       | 86.0 | 44.2   | 14.3  | 74.3  |




# Quantitation Results Report (QT Reviewed)


| Compound                 | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------------|---------|------|----------|-------|------|--------|-------|-------|
| trans-1,2-Dichloroethene | 25.4641 | 3.71 | -0.01    | 20706 | 61.0 | 152.1  | 123.9 | 183.9 |
|                          |         |      |          |       | 98.0 | 59.6   | 35.7  | 95.7  |

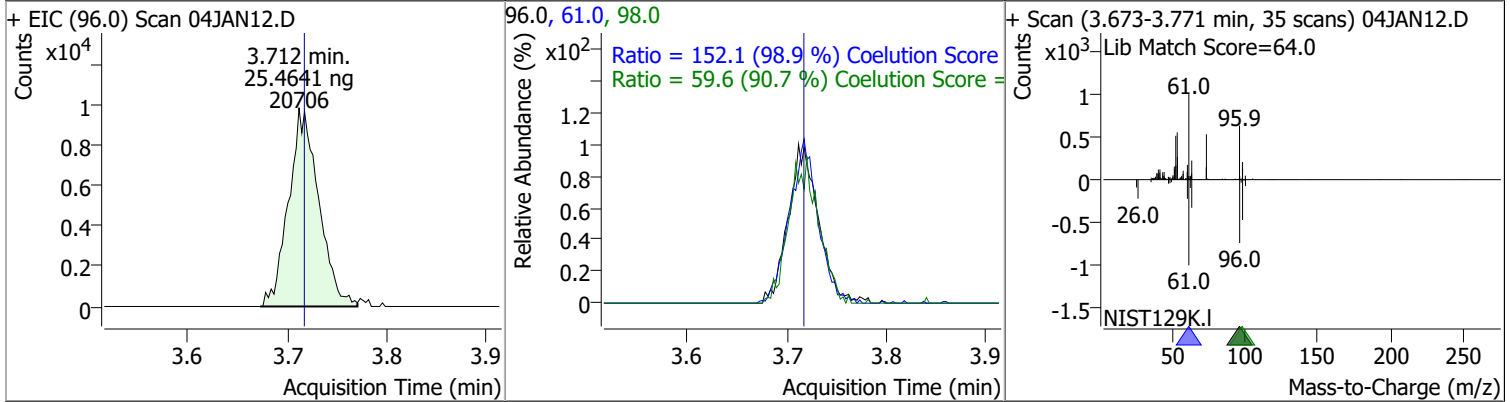

| Compound                       | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------------------|---------|------|----------|-------|------|--------|-------|-------|
| Methyl tert-butyl ether (MTBE) | 23.0418 | 3.75 | 0.00     | 24218 | 57.0 | 28.7   | 0.0   | 54.6  |

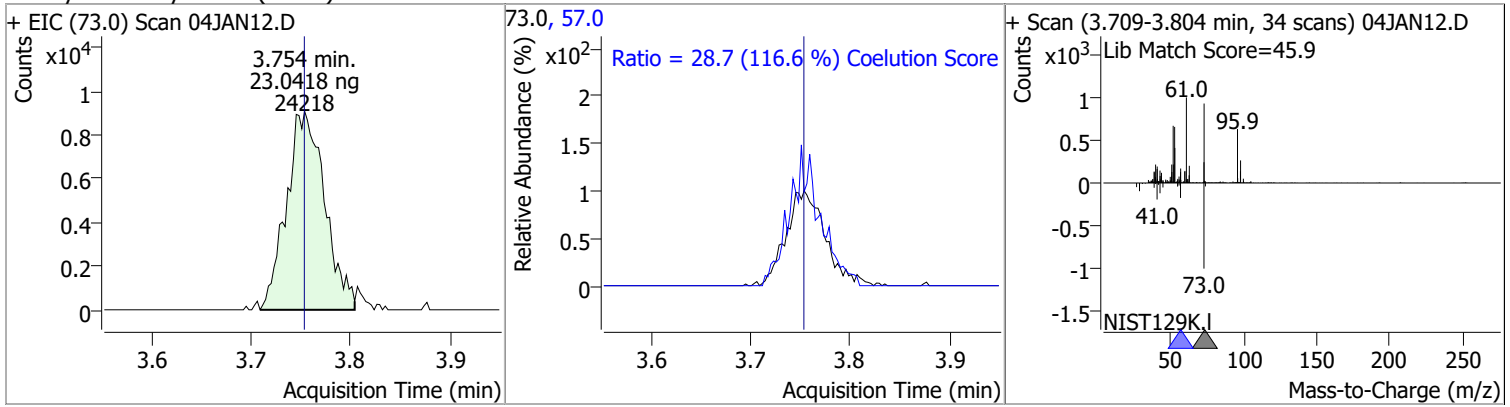


| Compound           | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|---------|------|----------|-------|------|--------|-------|-------|
| 1,1-Dichloroethane | 25.6835 | 4.38 | 0.00     | 38874 | 65.0 | 33.1   | 2.1   | 62.1  |
|                    |         |      |          |       | 83.0 | 11.5   | 0.0   | 43.7  |

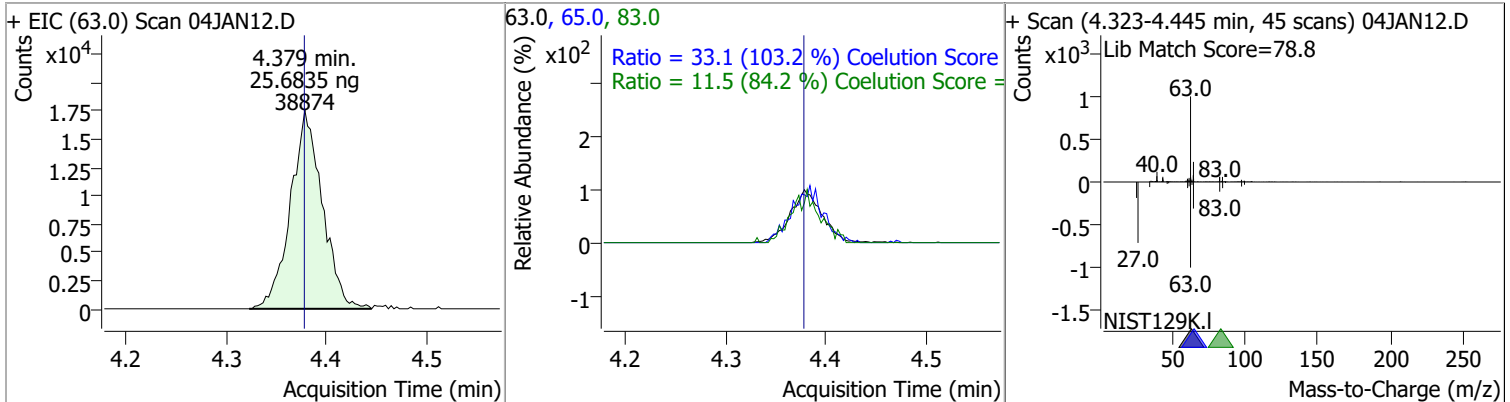


# Quantitation Results Report (QT Reviewed)


| Compound            | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|---------|------|----------|-------|------|--------|-------|-------|
| 2,2-Dichloropropane | 26.2692 | 5.19 | -0.01    | 29793 | 41.0 | 66.3   | 36.5  | 96.5  |
|                     |         |      |          |       | 97.0 | 23.4   | 0.0   | 53.2  |

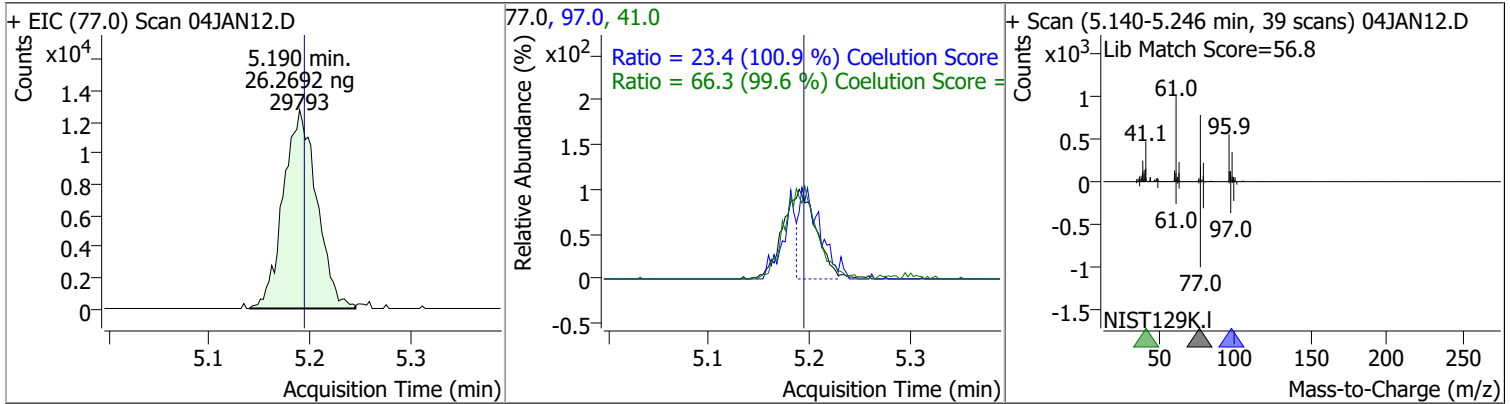


| Compound               | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|---------|------|----------|-------|------|--------|-------|-------|
| cis-1,2-Dichloroethene | 24.5653 | 5.21 | 0.00     | 20252 | 61.0 | 168.5  | 137.2 | 197.2 |
|                        |         |      |          |       | 98.0 | 64.9   | 37.3  | 97.3  |

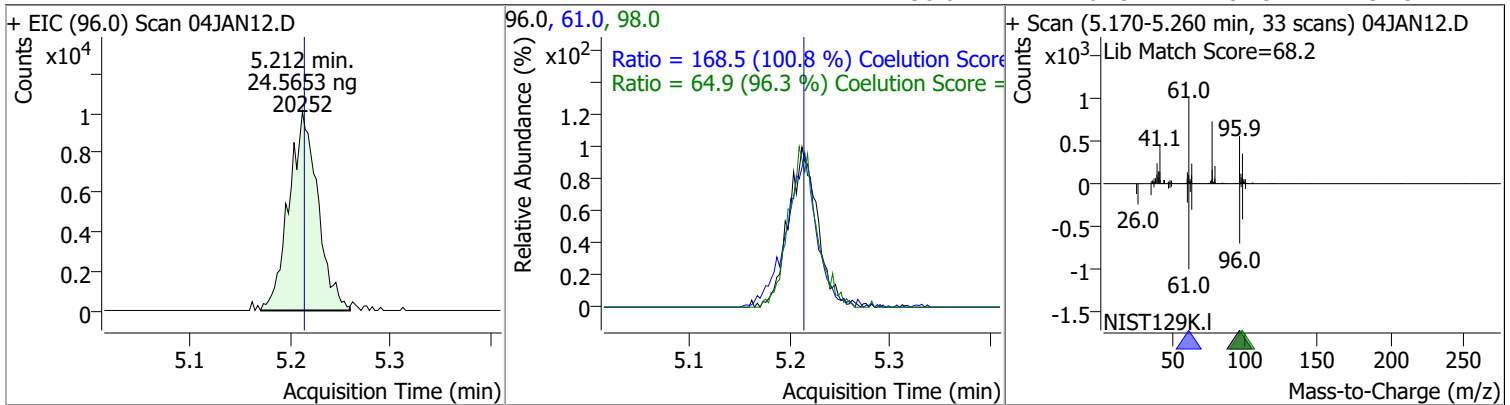

| Compound            | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|-------|------|--------|-------|-------|
| Methyl ethyl ketone | 235.0504 | 5.28 | 0.00     | 26248 | 72.0 | 20.4   | 0.0   | 51.3  |




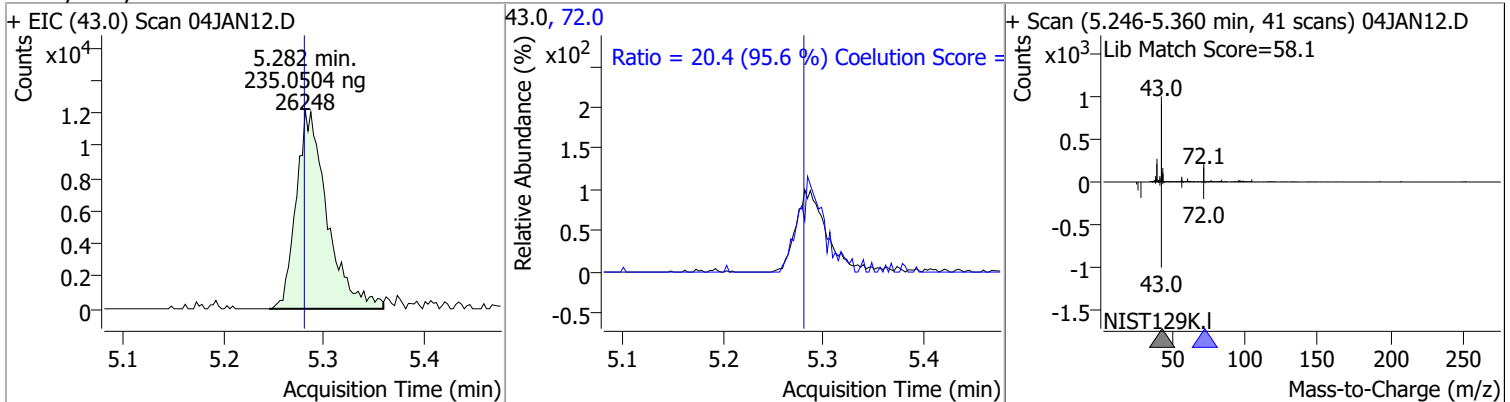


| Compound           | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|---------|------|----------|-------|------|--------|-------|-------|
| Bromochloromethane | 25.4383 | 5.52 | 0.00     | 8688  | 49.0 | 186.0  | 152.9 | 212.9 |

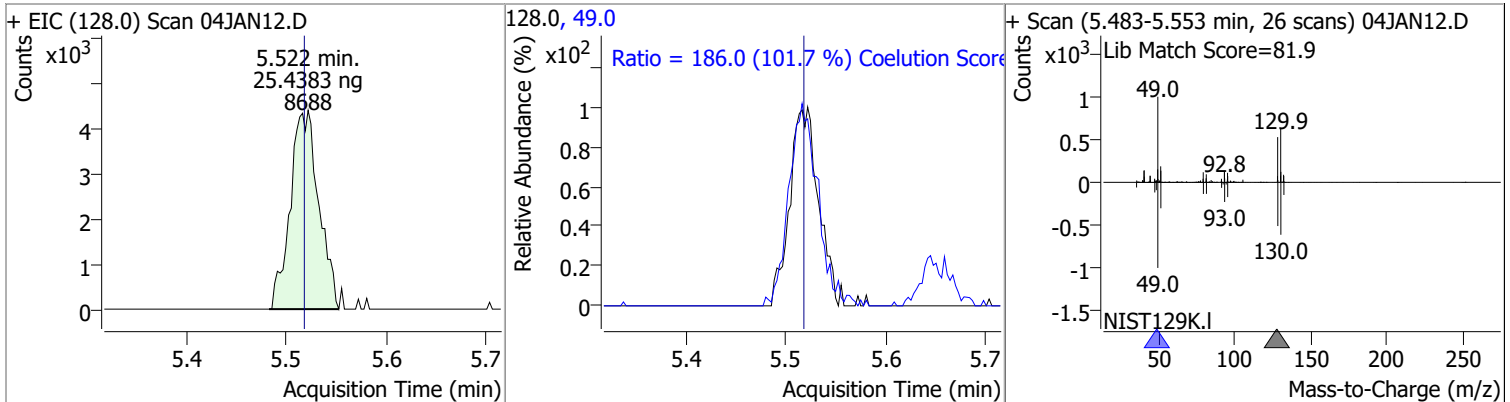




# Quantitation Results Report (QT Reviewed)

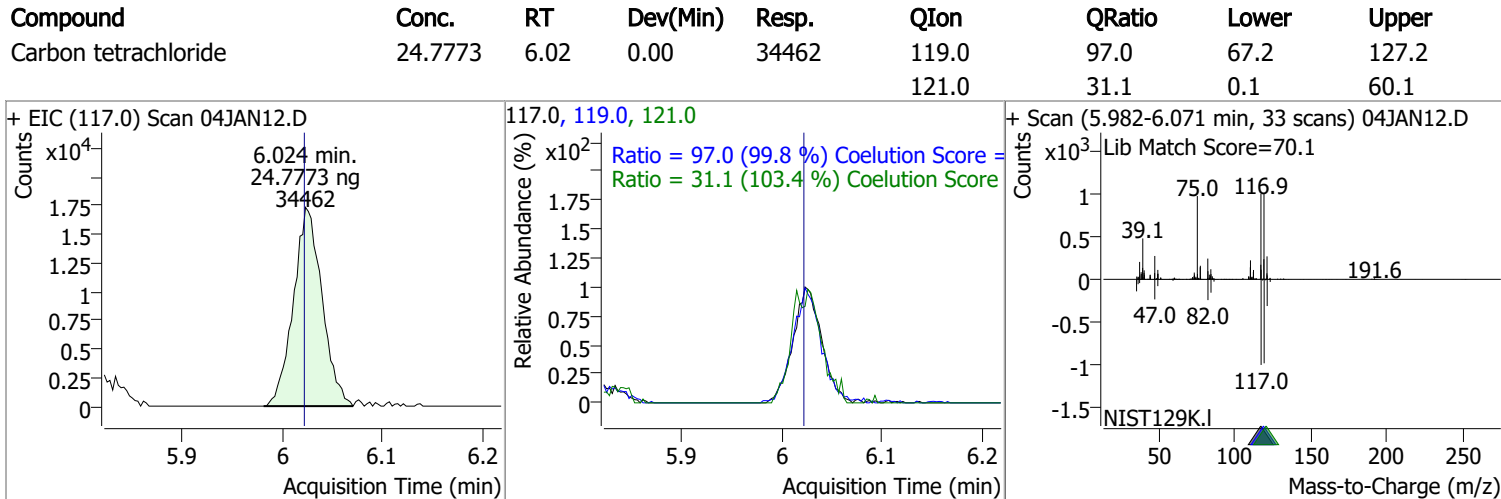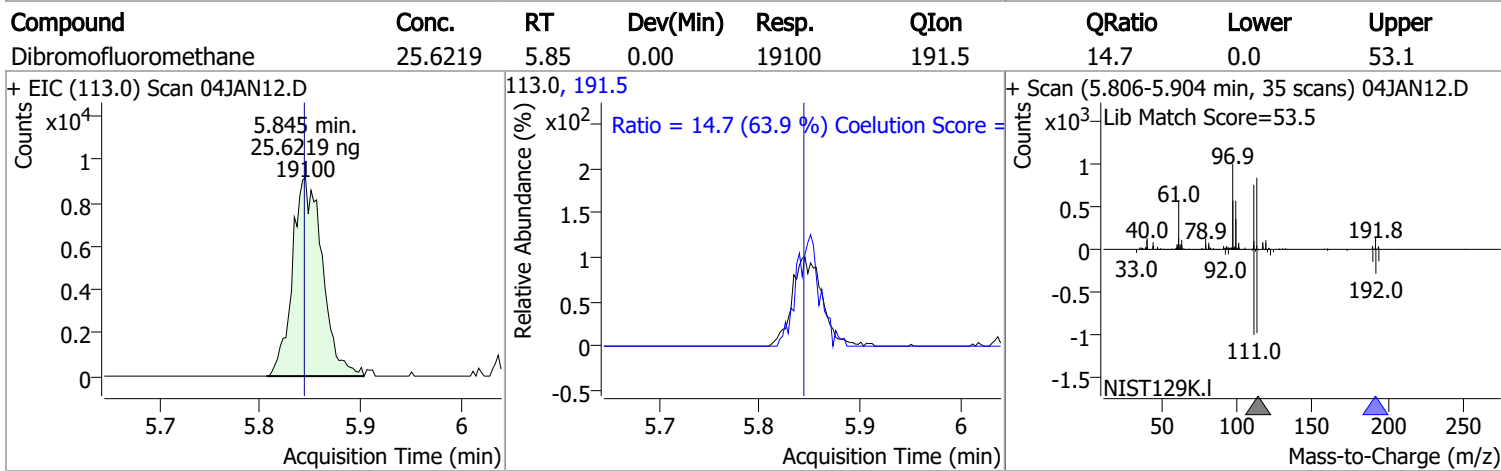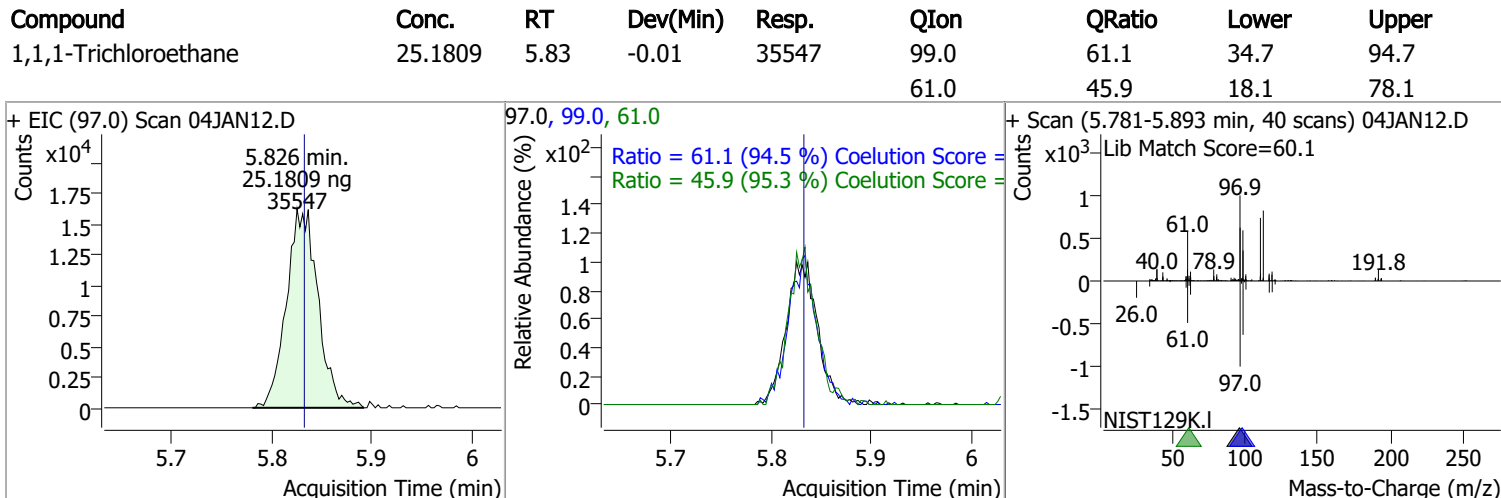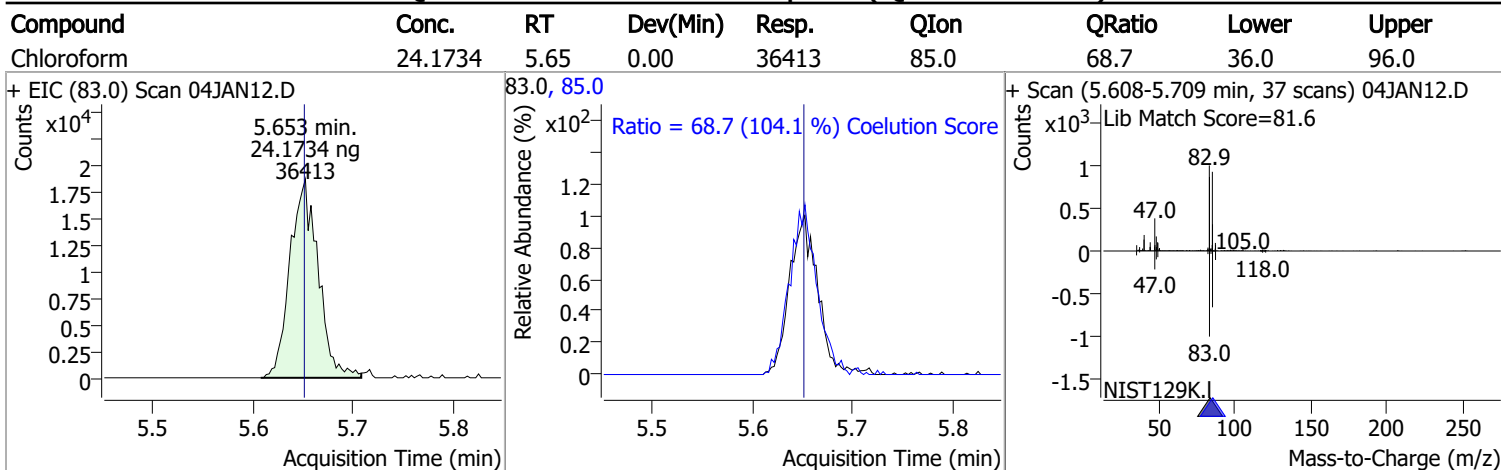


# Quantitation Results Report (QT Reviewed)


| Compound            | Conc.   | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|---------------------|---------|------|----------|-------|-------|--------|-------|-------|
| 1,1-Dichloropropene | 24.3617 | 6.04 | 0.00     | 29241 | 110.0 | 33.6   | 5.9   | 65.9  |
|                     |         |      |          |       | 77.0  | 31.9   | 0.1   | 60.1  |

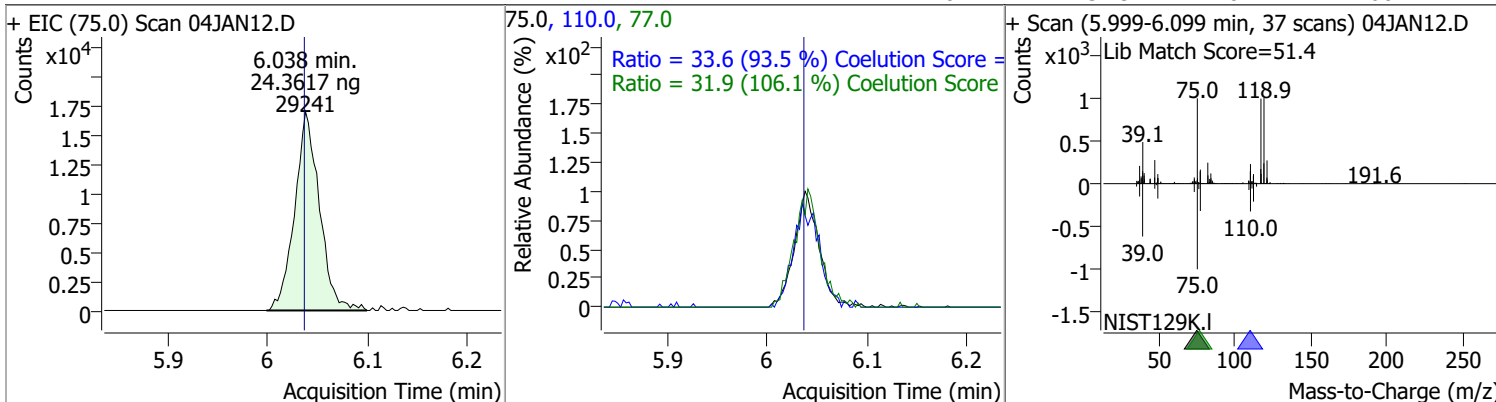


| Compound              | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|---------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 25.7280 | 6.24 | 0.00     | 8284  | 65.0 | 182.3  | 166.5 | 226.5 |



| Compound | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|---------|------|----------|-------|------|--------|-------|-------|
| Benzene  | 23.7919 | 6.28 | 0.00     | 74956 | 77.0 | 25.0   | 0.0   | 53.5  |

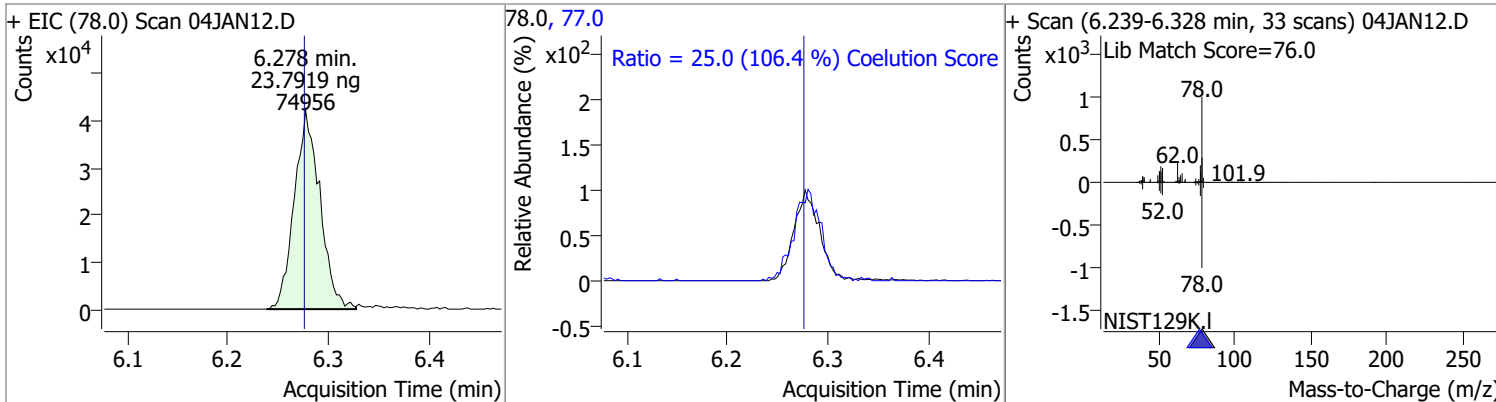


| Compound           | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|---------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane | 23.4616 | 6.32 | 0.00     | 19996 | 64.0 | 31.5   | 0.0   | 59.9  |
|                    |         |      |          |       | 98.0 | 8.3    | 0.0   | 37.6  |




# Quantitation Results Report (QT Reviewed)


| Compound        | Conc.   | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|-----------------|---------|------|----------|-------|-------|--------|-------|-------|
| Trichloroethene | 24.1484 | 7.03 | 0.00     | 21946 | 130.0 | 102.4  | 71.5  | 131.5 |
|                 |         |      |          |       | 97.0  | 67.5   | 34.1  | 94.1  |



| Compound            | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|---------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloropropane | 25.1147 | 7.27 | 0.00     | 20077 | 76.0 | 37.1   | 8.2   | 68.2  |




| Compound       | Conc.   | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|----------------|---------|------|----------|-------|-------|--------|-------|-------|
| Dibromomethane | 23.8439 | 7.39 | -0.01    | 8055  | 173.5 | 108.3  | 83.7  | 143.7 |
|                |         |      |          |       | 95.0  | 81.9   | 52.2  | 112.2 |




# Quantitation Results Report (QT Reviewed)


| Compound             | Conc.   | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|----------------------|---------|------|----------|-------|-------|--------|-------|-------|
| Bromodichloromethane | 24.3940 | 7.58 | 0.00     | 22743 | 85.0  | 66.3   | 34.5  | 94.5  |
|                      |         |      |          |       | 127.0 | 9.3    | 0.0   | 39.6  |

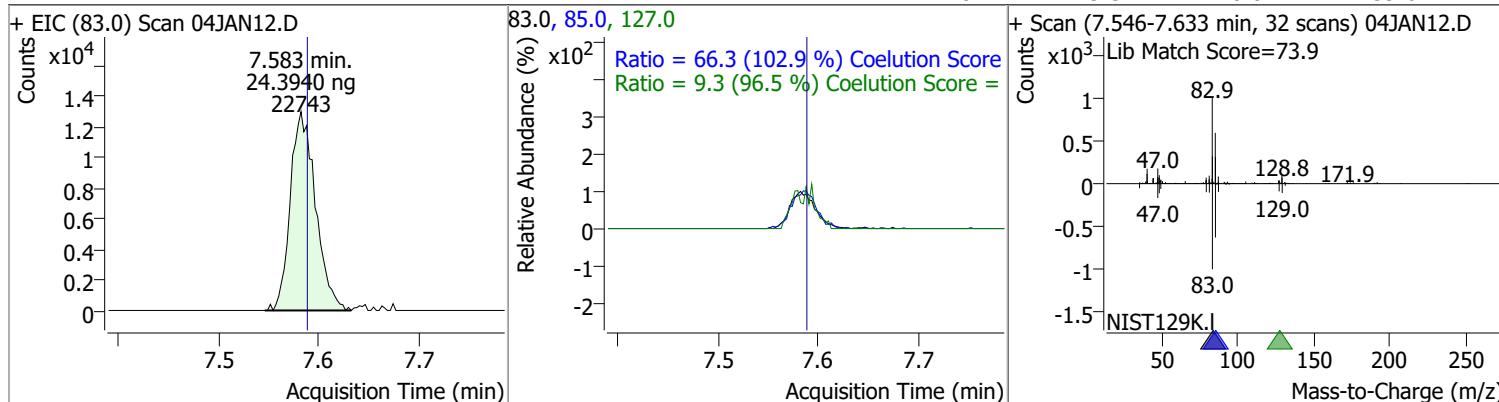

| Compound                | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------------|---------|------|----------|-------|------|--------|-------|-------|
| cis-1,3-Dichloropropene | 23.2528 | 8.06 | 0.00     | 24511 | 39.0 | 55.1   | 23.3  | 83.3  |
|                         |         |      |          |       | 77.0 | 33.2   | 1.0   | 61.0  |

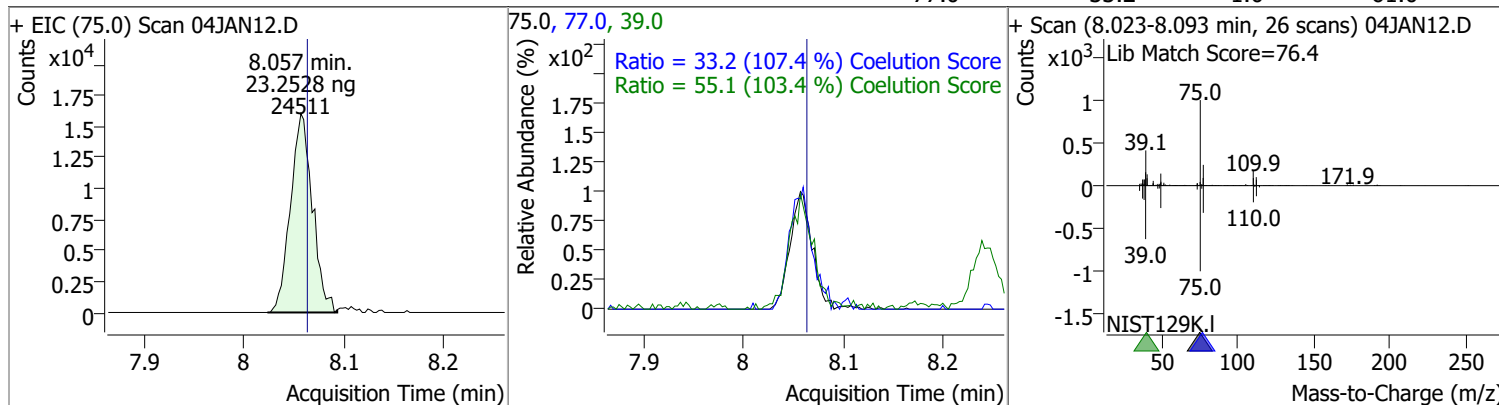

| Compound   | Conc.   | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|------------|---------|------|----------|-------|-------|--------|-------|-------|
| Toluene-d8 | 23.3046 | 8.32 | 0.00     | 67673 | 100.0 | 63.8   | 34.4  | 94.4  |
|            |         |      |          |       | 99.0  | 9.1    | 0.0   | 39.6  |

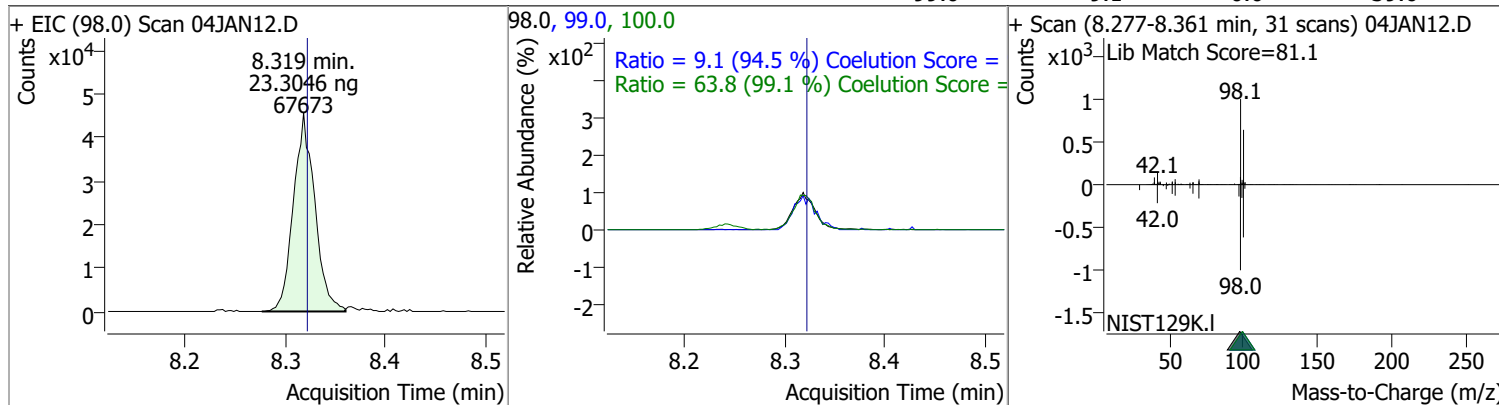


# Quantitation Results Report (QT Reviewed)


| Compound                    | Conc.   | RT   | Dev(Min)         | Resp. | QIon | QRatio                                       | Lower | Upper |
|-----------------------------|---------|------|------------------|-------|------|----------------------------------------------|-------|-------|
| Toluene                     | 23.6319 | 8.39 | 0.00             | 46355 | 91.0 | 174.6                                        | 145.8 | 205.8 |
| + EIC (92.0) Scan 04JAN12.D |         |      | 92.0, 91.0       |       |      | + Scan (8.350-8.450 min, 37 scans) 04JAN12.D |       |       |
|                             |         |      |                  |       |      |                                              |       |       |
| trans-1,3-Dichloropropene   | 23.7894 | 8.63 | 0.00             | 17850 | 39.0 | 55.9                                         | 23.4  | 83.4  |
| + EIC (75.0) Scan 04JAN12.D |         |      | 75.0, 77.0, 39.0 |       |      | + Scan (8.606-8.679 min, 27 scans) 04JAN12.D |       |       |
|                             |         |      |                  |       |      |                                              |       |       |
| 1,1,2-Trichloroethane       | 25.8400 | 8.82 | 0.00             | 10099 | 97.0 | 107.4                                        | 84.6  | 144.6 |
| + EIC (83.0) Scan 04JAN12.D |         |      | 83.0, 97.0, 85.0 |       |      | + Scan (8.785-8.857 min, 26 scans) 04JAN12.D |       |       |
|                             |         |      |                  |       |      |                                              |       |       |

# Quantitation Results Report (QT Reviewed)


| Compound          | Conc.   | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|-------------------|---------|------|----------|-------|-------|--------|-------|-------|
| Tetrachloroethene | 25.3948 | 8.94 | 0.00     | 20322 | 165.8 | 123.7  | 98.6  | 158.6 |
|                   |         |      |          |       | 129.0 | 90.9   | 61.5  | 121.5 |




| Compound            | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|---------|------|----------|-------|------|--------|-------|-------|
| 1,3-Dichloropropane | 24.3839 | 8.98 | 0.00     | 18745 | 78.0 | 33.6   | 2.9   | 62.9  |







| Compound             | Conc.   | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|----------------------|---------|------|----------|-------|-------|--------|-------|-------|
| Chlorodibromomethane | 24.3492 | 9.20 | -0.01    | 14873 | 127.0 | 78.7   | 48.0  | 108.0 |



| Compound          | Conc.   | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|-------------------|---------|------|----------|-------|-------|--------|-------|-------|
| 1,2-Dibromoethane | 24.3601 | 9.31 | 0.00     | 10410 | 109.0 | 89.3   | 64.5  | 124.5 |




# Quantitation Results Report (QT Reviewed)




# Quantitation Results Report (QT Reviewed)


| Compound | Conc.   | RT    | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|---------|-------|----------|-------|------|--------|-------|-------|
| o-Xylene | 23.6420 | 10.43 | 0.00     | 30463 | 91.0 | 210.5  | 183.1 | 243.1 |

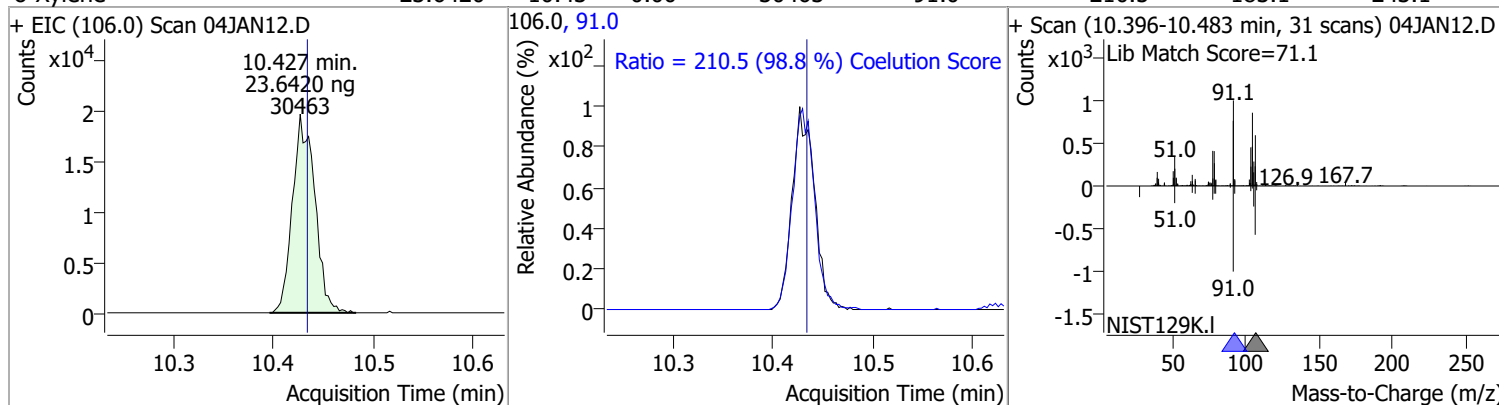


| Compound | Conc.   | RT    | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|---------|-------|----------|-------|------|--------|-------|-------|
| Styrene  | 23.4119 | 10.45 | 0.00     | 48569 | 78.0 | 51.8   | 19.6  | 79.6  |

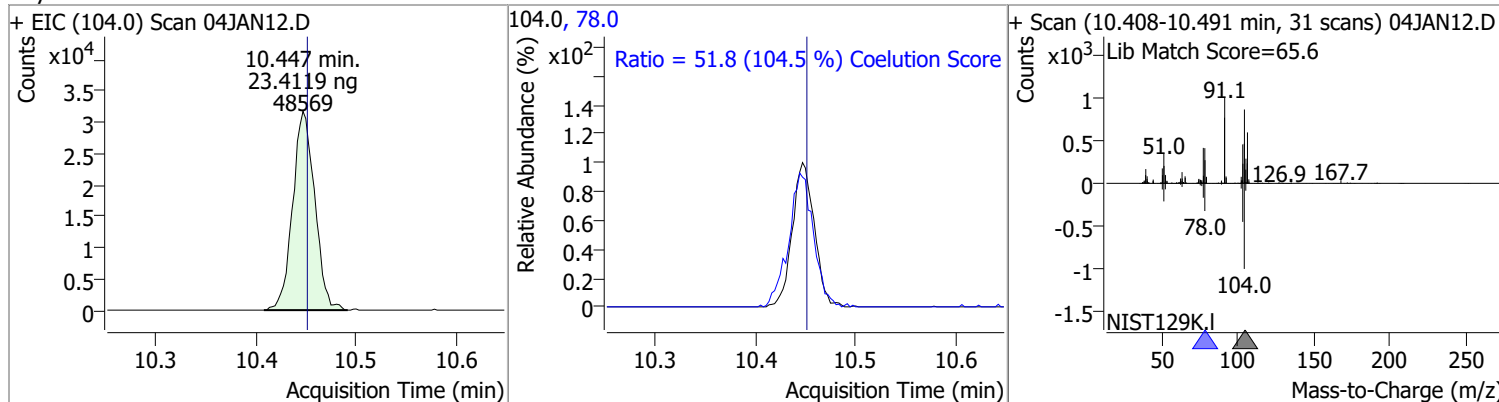

| Compound  | Conc.   | RT    | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|-----------|---------|-------|----------|-------|-------|--------|-------|-------|
| Bromoform | 25.9212 | 10.63 | 0.00     | 7972  | 170.5 | 47.6   | 22.1  | 82.1  |
|           |         |       |          |       | 174.5 | 50.7   | 20.1  | 80.1  |

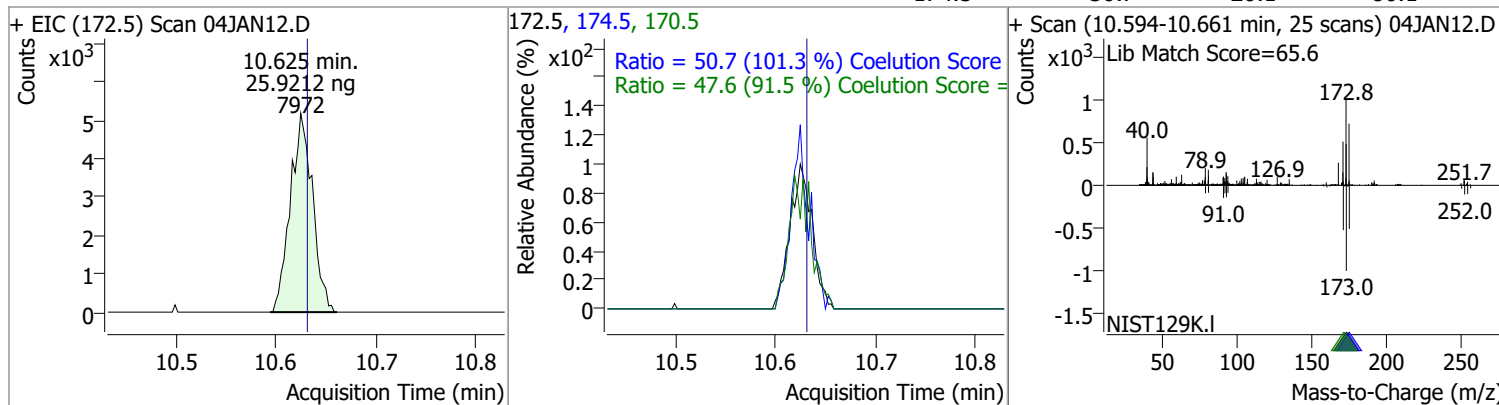


| Compound             | Conc.   | RT    | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|----------------------|---------|-------|----------|-------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 25.2899 | 10.95 | 0.00     | 22267 | 174.0 | 96.1   | 61.7  | 121.7 |
|                      |         |       |          |       | 176.0 | 89.8   | 60.6  | 120.6 |






# Quantitation Results Report (QT Reviewed)


| Compound     | Conc.   | RT    | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|--------------|---------|-------|----------|-------|-------|--------|-------|-------|
| Bromobenzene | 24.7613 | 11.09 | 0.00     | 19259 | 77.0  | 151.0  | 115.7 | 175.7 |
|              |         |       |          |       | 158.0 | 104.1  | 66.5  | 126.5 |

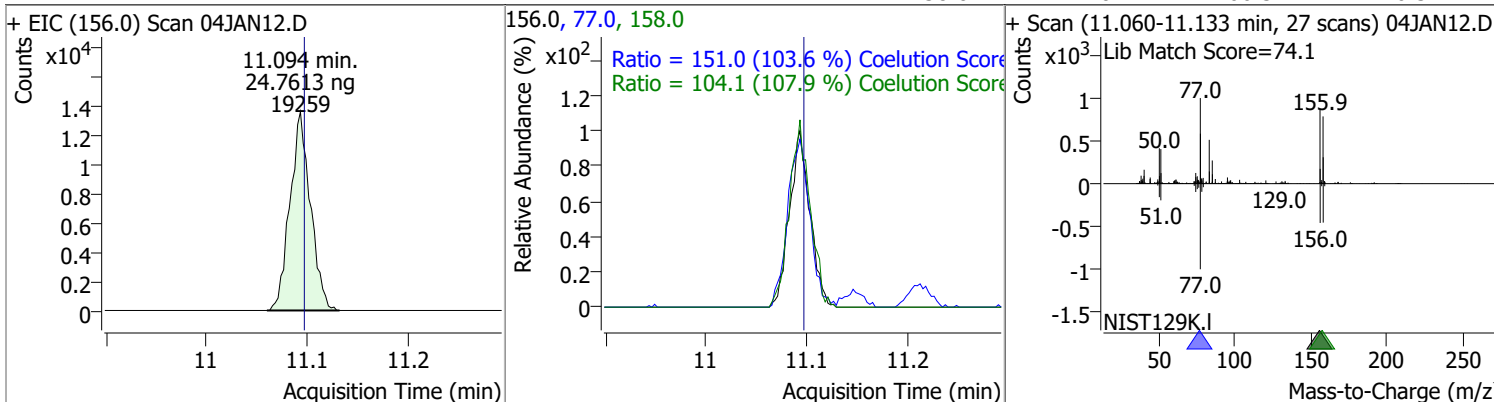


| Compound                  | Conc.   | RT    | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|---------|-------|----------|-------|------|--------|-------|-------|
| 1,1,2,2-Tetrachloroethane | 27.7883 | 11.11 | -0.01    | 12440 | 85.0 | 60.9   | 36.2  | 96.2  |



| Compound               | Conc.   | RT    | Dev(Min) | Resp.    | QIon  | QRatio | Lower | Upper |
|------------------------|---------|-------|----------|----------|-------|--------|-------|-------|
| 1,2,3-Trichloropropane | 26.7144 | 11.15 | 0.00     | 3200 (m) | 112.0 | 66.8   | 33.5  | 93.5  |



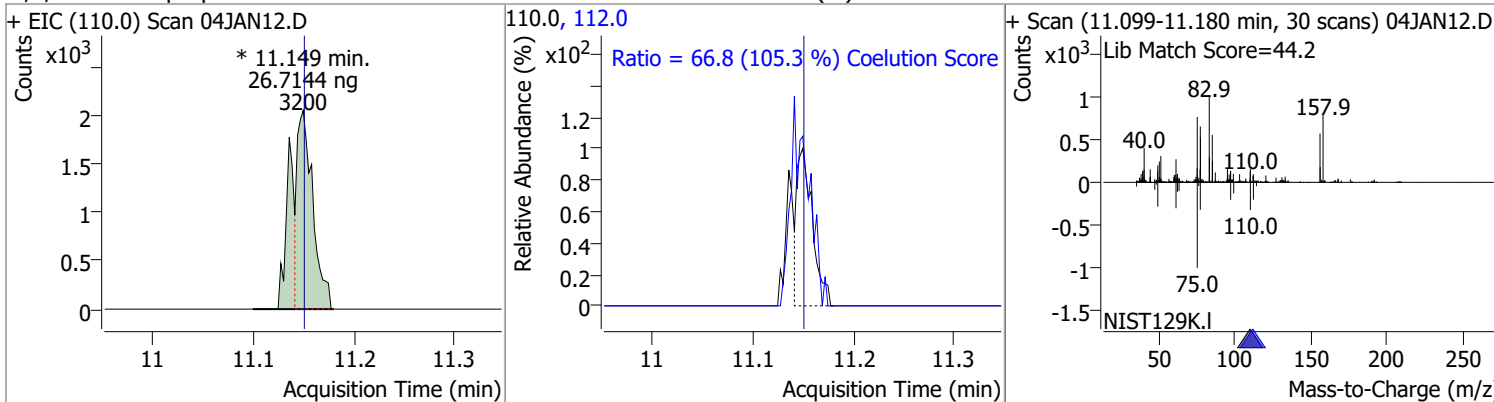


| Compound        | Conc.   | RT    | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|---------|-------|----------|-------|------|--------|-------|-------|
| 2-Chlorotoluene | 25.0550 | 11.29 | -0.01    | 19390 | 91.0 | 270.4  | 252.3 | 312.3 |






# Quantitation Results Report (QT Reviewed)




| Compound        | Conc.   | RT    | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|-----------------|---------|-------|----------|-------|-------|--------|-------|-------|
| 4-Chlorotoluene | 24.3936 | 11.40 | 0.00     | 61551 | 126.0 | 31.8   | 1.7   | 61.7  |

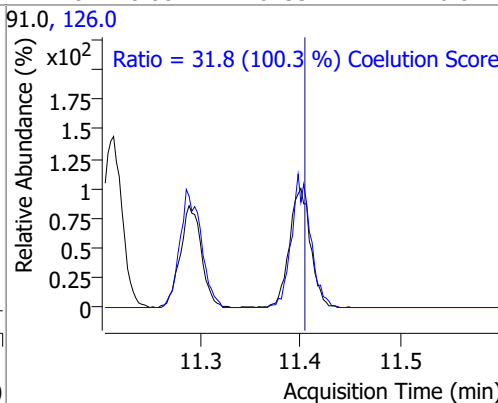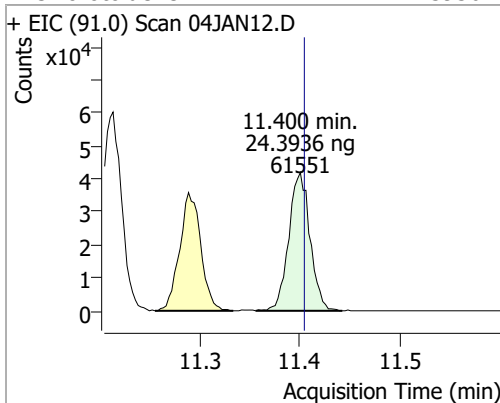

| Compound            | Conc.   | RT    | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|---------------------|---------|-------|----------|-------|-------|--------|-------|-------|
| 1,3-Dichlorobenzene | 25.7725 | 12.03 | 0.00     | 36559 | 148.0 | 61.3   | 33.6  | 93.6  |
|                     |         |       |          |       | 111.0 | 38.2   | 9.8   | 69.8  |


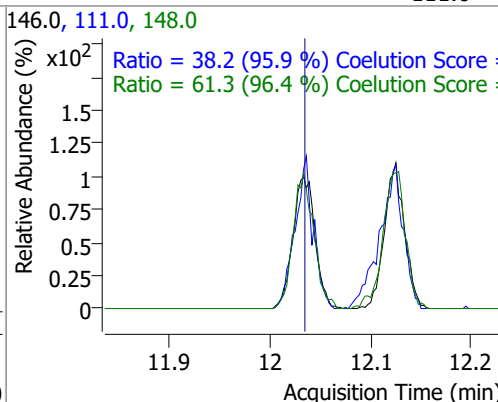
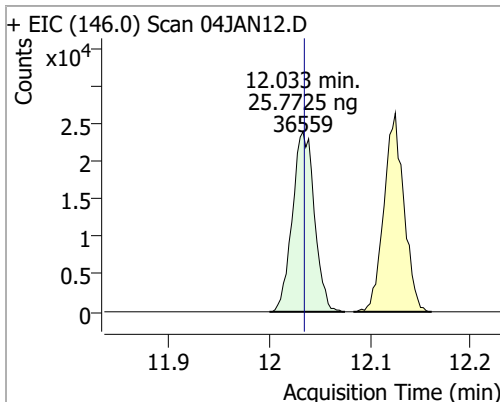


| Compound            | Conc.   | RT    | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|---------------------|---------|-------|----------|-------|-------|--------|-------|-------|
| 1,4-Dichlorobenzene | 25.3284 | 12.13 | 0.00     | 36635 | 148.0 | 67.6   | 33.1  | 93.1  |
|                     |         |       |          |       | 111.0 | 46.4   | 9.1   | 69.1  |

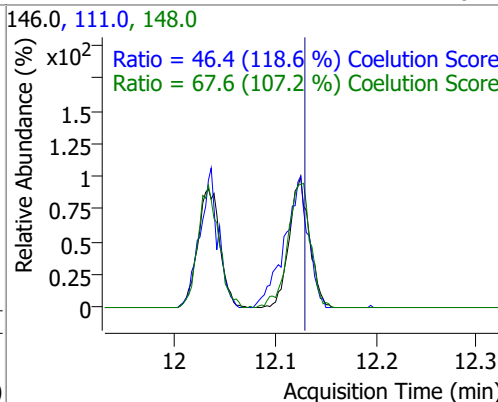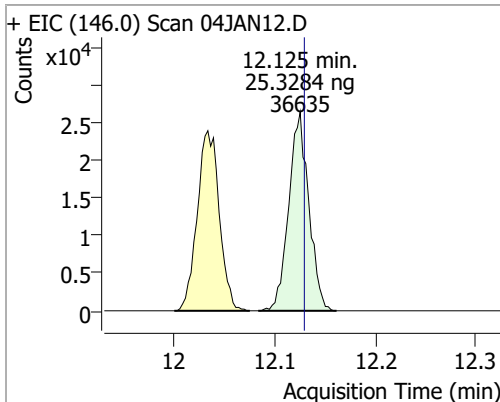


# Quantitation Results Report (QT Reviewed)

| Compound            | Conc.   | RT    | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|---------------------|---------|-------|----------|-------|-------|--------|-------|-------|
| 1,2-Dichlorobenzene | 24.9402 | 12.49 | -0.01    | 29899 | 148.0 | 62.9   | 33.9  | 93.9  |
|                     |         |       |          |       | 111.0 | 42.3   | 11.0  | 71.0  |

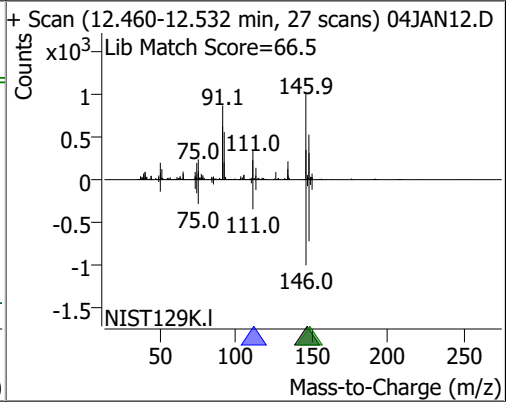

# Quantitation Results Report (QT Reviewed)

|                |                                     |                   |                       |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File      | 04JAN13.D                           | Operator          | MSC                   |
| Acq. Method    | 5975CACQF.M                         | Acq. Date-Time    | 1/4/2022 4:55:32 PM   |
| Sample Name    | ICAL010422_4                        | Instrument        | VOA5975C              |
| Vial           | 13                                  | Multiplier        | 1.00                  |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m  | Comment           |                       |
| Tune File      | BFB_Atune3.u                        | Tune Date         | 10/11/2021 4:02:00 PM |
| Batch Name     | VG010422_8260B.batch.bin            | Last Calib Update | 1/9/2022 8:59:52 PM   |
| Ref Library    | \\MASSHUNTER\Org\Library\NIST129K.I |                   |                       |















| Compound                           | RT                   | QIon  | Resp.  | Conc.             | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|-------------------|-------|----------|
| <b>Internal Standards</b>          |                      |       |        |                   |       |          |
| M Fluorobenzene                    | 6.623                | 96.0  | 778120 | 250.0000          | ng    | 0.000    |
| M Chlorobenzene-d5                 | 9.774                | 82.0  | 300356 | 250.0000          | ng    | 0.003    |
| M 1,4-Dichlorobenzene-d4           | 12.100               | 152.0 | 248636 | 250.0000          | ng    | 0.000    |
| <b>System Monitoring Compounds</b> |                      |       |        |                   |       |          |
| S Dibromofluoromethane             | 5.848                | 113.0 | 35309  | 48.1661           | ng    | 0.003    |
| Spiked Amount: 250.000             | Range: 80.0 - 119.0% |       |        | Recovery = 19.27% |       | *        |
| S 1,2-Dichloroethane-d4            | 6.233                | 67.0  | 15238  | 48.1252           | ng    | 0.000    |
| Spiked Amount: 250.000             | Range: 81.0 - 118.0% |       |        | Recovery = 19.25% |       | *        |
| S Toluene-d8                       | 8.319                | 98.0  | 136453 | 47.1441           | ng    | 0.000    |
| Spiked Amount: 250.000             | Range: 89.0 - 112.0% |       |        | Recovery = 18.86% |       | *        |
| S p-Bromofluorobenzene             | 10.951               | 95.0  | 42506  | 46.6647           | ng    | -0.003   |
| Spiked Amount: 250.000             | Range: 85.0 - 114.0% |       |        | Recovery = 18.67% |       | *        |
| <b>Target Compounds</b>            |                      |       |        |                   |       |          |
| T Dichlorodifluoromethane          | 1.241                | 85.0  | 50457  | 49.4835           | ng    | 97       |
| T Chloromethane                    | 1.408                | 50.0  | 61632  | 49.7983           | ng    | 99       |
| T Vinyl chloride                   | 1.495                | 62.0  | 54521  | 48.9580           | ng    | 96       |
| T Bromomethane                     | 1.799                | 96.0  | 23699  | 47.5921           | ng    | 100      |
| T Chloroethane                     | 1.897                | 64.0  | 25484  | 46.2243           | ng    | 98       |
| T Trichlorofluoromethane           | 2.145                | 101.0 | 68163  | 49.3128           | ng    | 98       |
| T 1,1-Dichloroethene               | 2.702                | 96.0  | 38253  | 48.8056           | ng    | 100      |
| T Methylene chloride               | 3.335                | 49.0  | 58282  | 50.4421           | ng    | 99       |
| T trans-1,2-Dichloroethene         | 3.717                | 96.0  | 39596  | 49.5178           | ng    | 99       |
| T Methyl tert-butyl ether (MTBE)   | 3.757                | 73.0  | 49126  | 47.5301           | ng    | 100      |
| T 1,1-Dichloroethane               | 4.381                | 63.0  | 73205  | 49.1828           | ng    | 100      |
| T 2,2-Dichloropropane              | 5.193                | 77.0  | 56189  | 50.3804           | ng    | 100      |
| T cis-1,2-Dichloroethene           | 5.209                | 96.0  | 39251  | 48.4154           | ng    | 99       |
| T Methyl ethyl ketone              | 5.285                | 43.0  | 52648  | 479.4296          | ng    | 99       |
| T Bromochloromethane               | 5.516                | 128.0 | 17338  | 51.6233           | ng    | 96       |
| T Chloroform                       | 5.650                | 83.0  | 71403  | 48.2031           | ng    | 99       |

# Quantitation Results Report (QT Reviewed)

| Compound                    | RT     | QIon  | Resp.  | Conc.   | Units | Dev(Min) |
|-----------------------------|--------|-------|--------|---------|-------|----------|
| T 1,1,1-Trichloroethane     | 5.834  | 97.0  | 67007  | 48.2688 | ng    | 98       |
| T Carbon tetrachloride      | 6.026  | 117.0 | 65313  | 47.7520 | ng    | 98       |
| T 1,1-Dichloropropene       | 6.035  | 75.0  | 56376  | 47.7627 | ng    | 99       |
| T Benzene                   | 6.277  | 78.0  | 148727 | 48.0054 | ng    | 100      |
| T 1,2-Dichloroethane        | 6.325  | 62.0  | 41058  | 48.9880 | ng    | 97       |
| T Trichloroethene           | 7.030  | 95.0  | 42682  | 47.1189 | ng    | 98       |
| T 1,2-Dichloropropane       | 7.273  | 63.0  | 37870  | 47.5273 | ng    | 96       |
| T Dibromomethane            | 7.396  | 93.0  | 15989  | 47.4844 | ng    | 97       |
| T Bromodichloromethane      | 7.585  | 83.0  | 43900  | 47.2409 | ng    | 97       |
| T cis-1,3-Dichloropropene   | 8.057  | 75.0  | 48886  | 46.5283 | ng    | 97       |
| T Toluene                   | 8.388  | 92.0  | 91915  | 47.0116 | ng    | 100      |
| T trans-1,3-Dichloropropene | 8.639  | 75.0  | 35179  | 47.0378 | ng    | 100      |
| T 1,1,2-Trichloroethane     | 8.815  | 83.0  | 18884  | 48.4759 | ng    | 99       |
| T Tetrachloroethene         | 8.935  | 163.8 | 36925  | 46.2932 | ng    | 97       |
| T 1,3-Dichloropropane       | 8.980  | 76.0  | 37457  | 48.8841 | ng    | 98       |
| T Chlorodibromomethane      | 9.203  | 129.0 | 28153  | 46.2411 | ng    | 99       |
| T 1,2-Dibromoethane         | 9.303  | 107.0 | 21037  | 49.3889 | ng    | 93       |
| T Chlorobenzene             | 9.802  | 112.0 | 101452 | 47.3959 | ng    | 99       |
| T 1,1,1,2-Tetrachloroethane | 9.889  | 131.0 | 35544  | 47.5029 | ng    | 99       |
| T Ethylbenzene              | 9.917  | 91.0  | 173769 | 46.8079 | ng    | 99       |
| T m+p-Xylenes               | 10.039 | 106.0 | 133498 | 92.5347 | ng    | 98       |
| T o-Xylene                  | 10.430 | 106.0 | 61016  | 47.5086 | ng    | 98       |
| T Styrene                   | 10.444 | 104.0 | 96576  | 46.7052 | ng    | 100      |
| T Bromoform                 | 10.625 | 172.5 | 16073  | 50.5170 | ng    | 96       |
| T Bromobenzene              | 11.093 | 156.0 | 38282  | 47.5759 | ng    | 98       |
| T 1,1,2,2-Tetrachloroethane | 11.105 | 83.0  | 22514  | 48.6124 | ng    | 99       |
| T 1,2,3-Trichloropropane    | 11.146 | 110.0 | 6096   | 49.1924 | ng    | 97       |
| T 2-Chlorotoluene           | 11.289 | 126.0 | 37987  | 47.4466 | ng    | 99       |
| T 4-Chlorotoluene           | 11.400 | 91.0  | 126308 | 48.3865 | ng    | 100      |
| T 1,3-Dichlorobenzene       | 12.033 | 146.0 | 69539  | 47.3853 | ng    | 99       |
| T 1,4-Dichlorobenzene       | 12.125 | 146.0 | 71841  | 48.0106 | ng    | 97       |
| T 1,2-Dichlorobenzene       | 12.491 | 146.0 | 60213  | 48.5498 | ng    | 98       |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (\*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

# Quantitation Results Report (QT Reviewed)

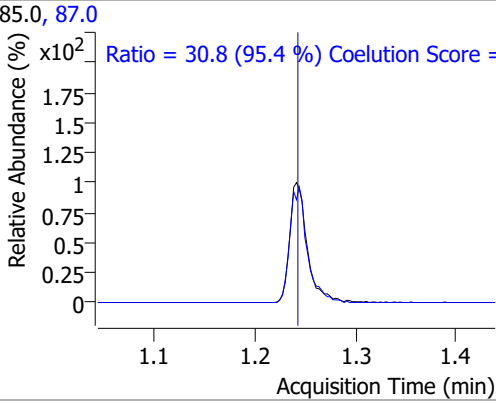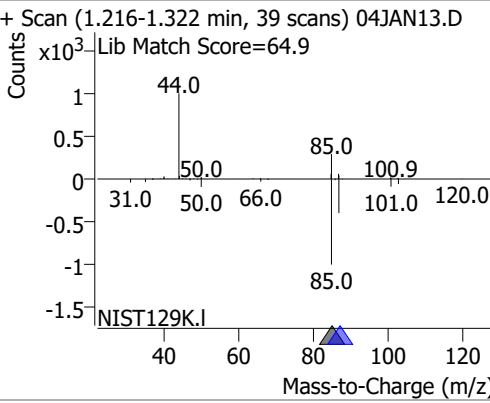
| Compound                                                                                                          | Conc.   | RT   | Dev(Min)                                                                                           | Resp. | QIon | QRatio                                                                                                                                                        | Lower | Upper |
|-------------------------------------------------------------------------------------------------------------------|---------|------|----------------------------------------------------------------------------------------------------|-------|------|---------------------------------------------------------------------------------------------------------------------------------------------------------------|-------|-------|
| Dichlorodifluoromethane                                                                                           | 49.4835 | 1.24 | 0.00                                                                                               | 50457 | 87.0 | 30.8                                                                                                                                                          | 2.3   | 62.3  |
| + EIC (85.0) Scan 04JAN13.D<br>   |         |      | 85.0, 87.0<br>   |       |      | + Scan (1.216-1.322 min, 39 scans) 04JAN13.D<br>Lib Match Score=64.9<br>   |       |       |
| Chloromethane                                                                                                     | 49.7983 | 1.41 | 0.00                                                                                               | 61632 | 52.0 | 32.8                                                                                                                                                          | 2.1   | 62.1  |
| + EIC (50.0) Scan 04JAN13.D<br>  |         |      | 50.0, 52.0<br>  |       |      | + Scan (1.372-1.478 min, 39 scans) 04JAN13.D<br>Lib Match Score=58.0<br>  |       |       |
| Vinyl chloride                                                                                                    | 48.9580 | 1.49 | 0.00                                                                                               | 54521 | 64.0 | 27.7                                                                                                                                                          | 0.0   | 59.9  |
| + EIC (62.0) Scan 04JAN13.D<br> |         |      | 62.0, 64.0<br> |       |      | + Scan (1.470-1.570 min, 37 scans) 04JAN13.D<br>Lib Match Score=70.1<br> |       |       |
| Bromomethane                                                                                                      | 47.5921 | 1.80 | 0.00                                                                                               | 23699 | 94.0 | 104.9                                                                                                                                                         | 74.6  | 134.6 |
| + EIC (96.0) Scan 04JAN13.D<br> |         |      | 96.0, 94.0<br> |       |      | + Scan (1.768-1.855 min, 32 scans) 04JAN13.D<br>Lib Match Score=73.7<br> |       |       |

# Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|-------|----|----------|-------|------|--------|-------|-------|
|----------|-------|----|----------|-------|------|--------|-------|-------|




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|-------|----|----------|-------|------|--------|-------|-------|
|----------|-------|----|----------|-------|------|--------|-------|-------|

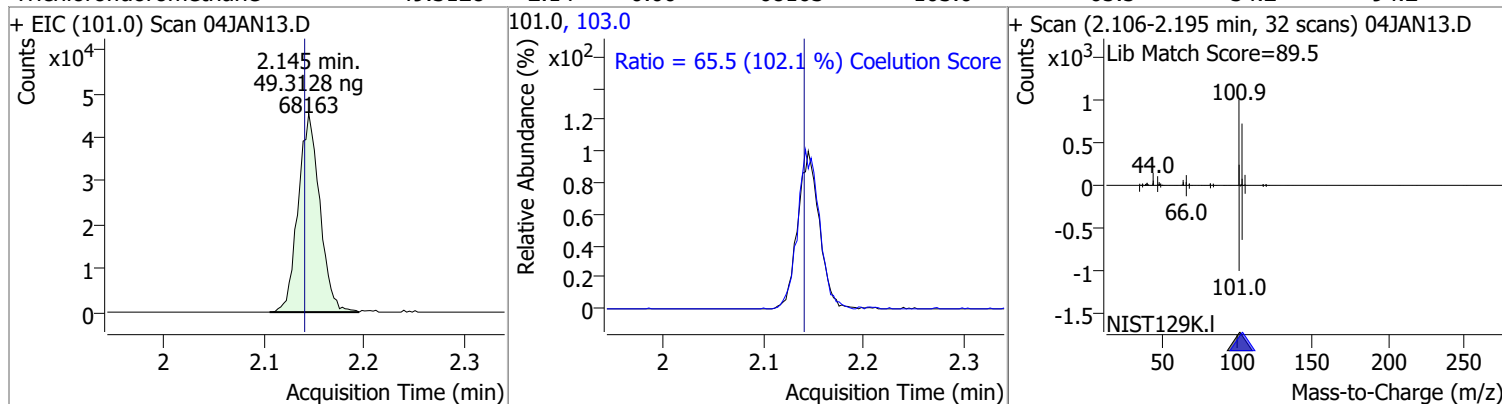

| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|-------|----|----------|-------|------|--------|-------|-------|
|----------|-------|----|----------|-------|------|--------|-------|-------|

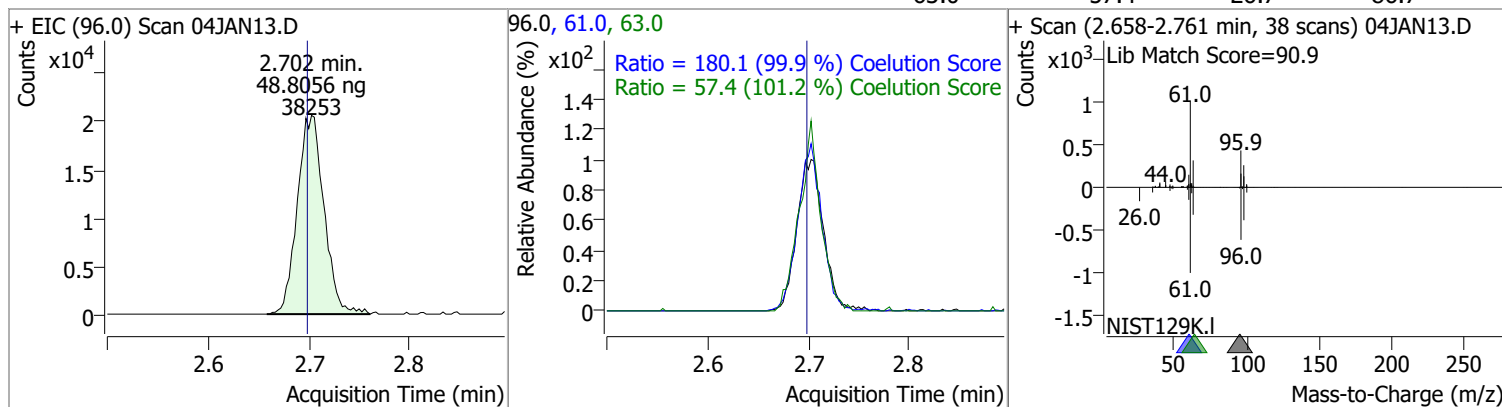


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|-------|----|----------|-------|------|--------|-------|-------|
|----------|-------|----|----------|-------|------|--------|-------|-------|

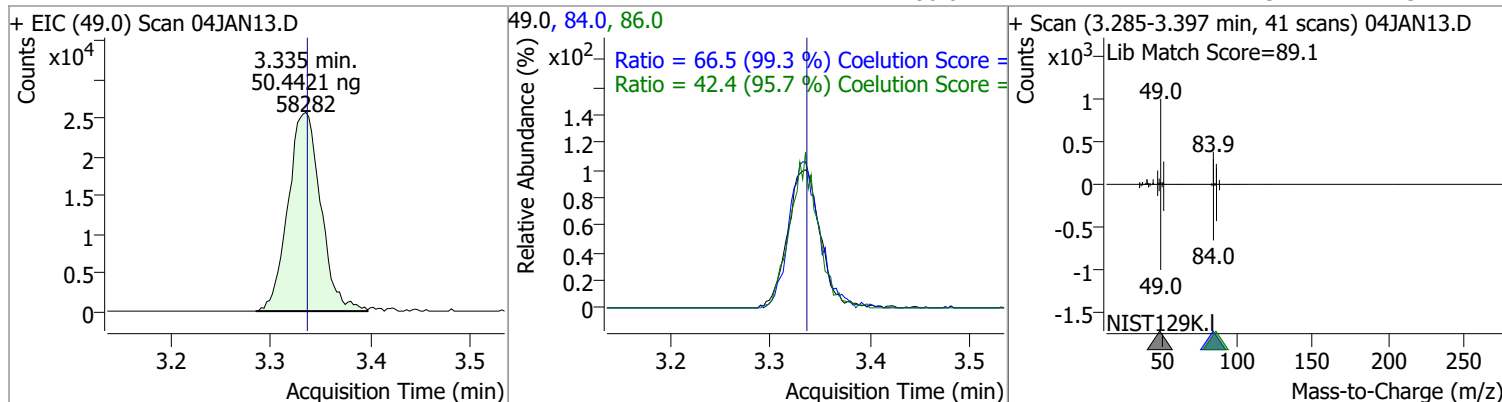


# Quantitation Results Report (QT Reviewed)


| Compound                 | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------------|---------|------|----------|-------|------|--------|-------|-------|
| trans-1,2-Dichloroethene | 49.5178 | 3.72 | 0.00     | 39596 | 61.0 | 152.1  | 123.9 | 183.9 |
|                          |         |      |          |       | 98.0 | 65.3   | 35.7  | 95.7  |



| Compound                       | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------------------|---------|------|----------|-------|------|--------|-------|-------|
| Methyl tert-butyl ether (MTBE) | 47.5301 | 3.76 | 0.00     | 49126 | 57.0 | 24.8   | 0.0   | 54.6  |

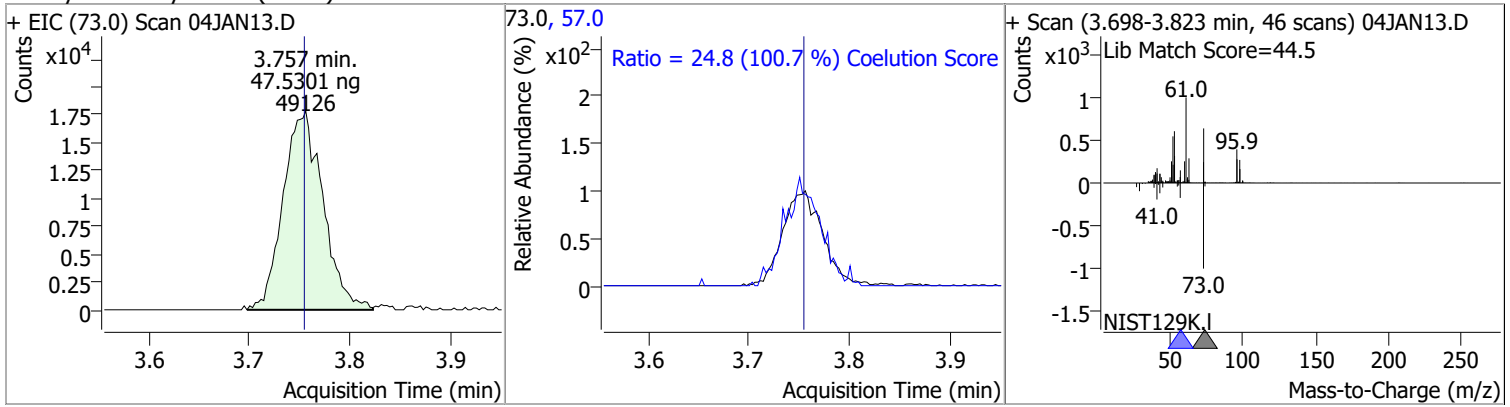


| Compound           | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|---------|------|----------|-------|------|--------|-------|-------|
| 1,1-Dichloroethane | 49.1828 | 4.38 | 0.00     | 73205 | 65.0 | 32.2   | 2.1   | 62.1  |
|                    |         |      |          |       | 83.0 | 13.7   | 0.0   | 43.7  |

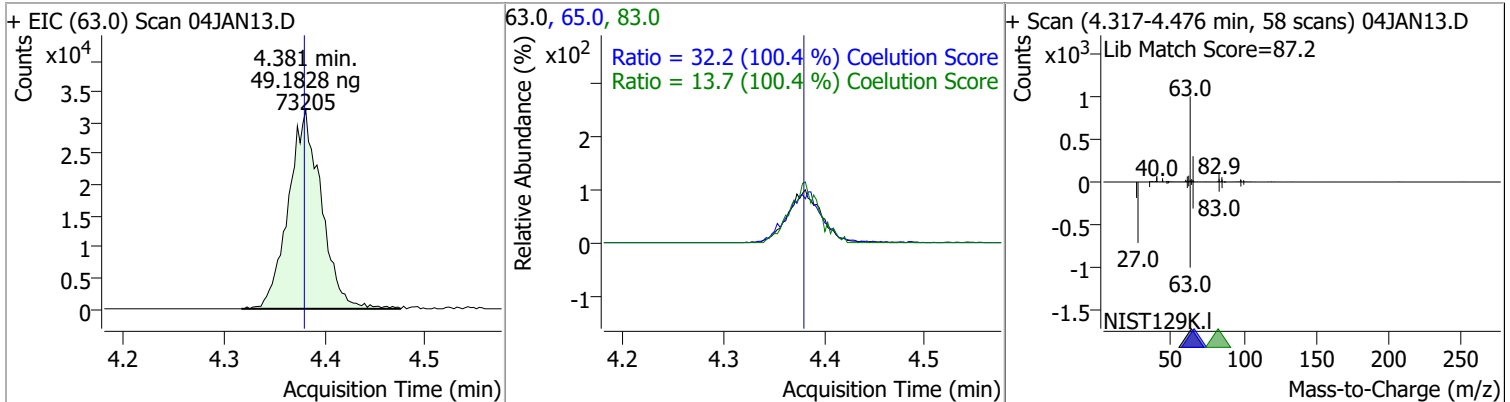




# Quantitation Results Report (QT Reviewed)


| Compound            | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|---------|------|----------|-------|------|--------|-------|-------|
| 2,2-Dichloropropane | 50.3804 | 5.19 | 0.00     | 56189 | 41.0 | 66.6   | 36.5  | 96.5  |
|                     |         |      |          |       | 97.0 | 23.3   | 0.0   | 53.2  |

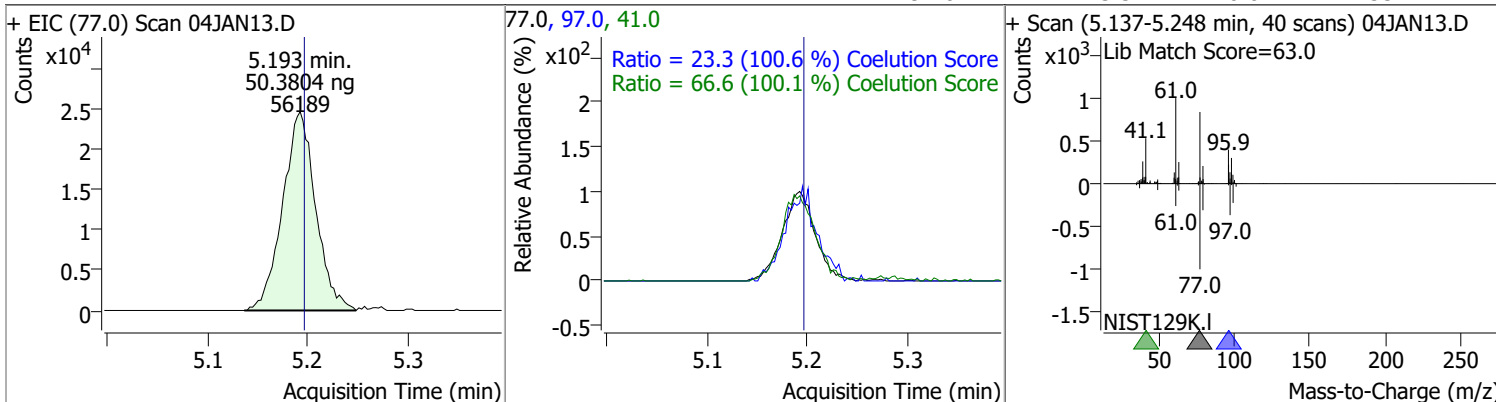


| Compound               | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------------------|---------|------|----------|-------|------|--------|-------|-------|
| cis-1,2-Dichloroethene | 48.4154 | 5.21 | -0.01    | 39251 | 61.0 | 167.9  | 137.2 | 197.2 |
|                        |         |      |          |       | 98.0 | 66.0   | 37.3  | 97.3  |

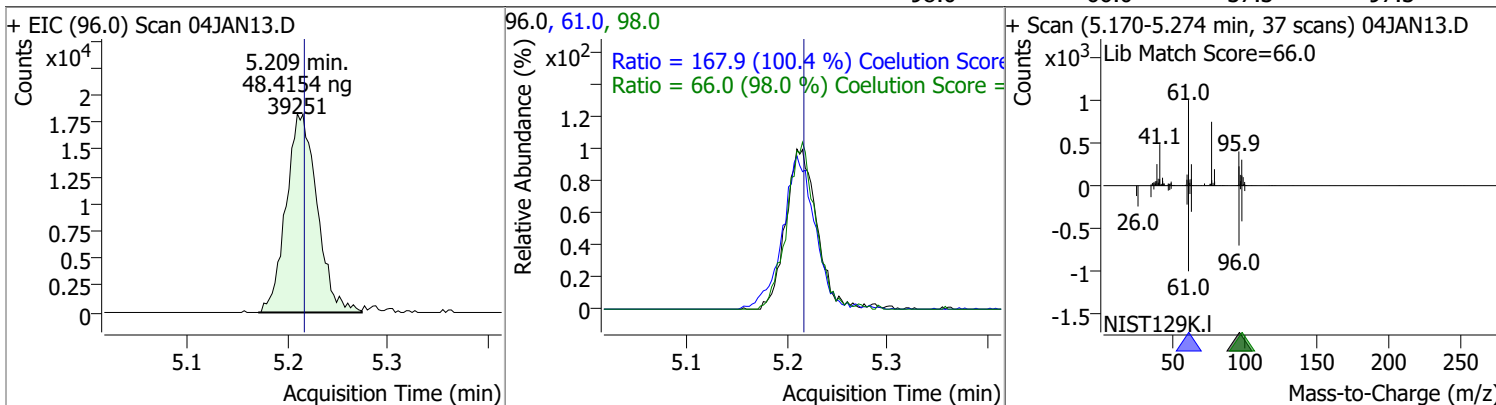

| Compound            | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|-------|------|--------|-------|-------|
| Methyl ethyl ketone | 479.4296 | 5.28 | 0.00     | 52648 | 72.0 | 20.6   | 0.0   | 51.3  |

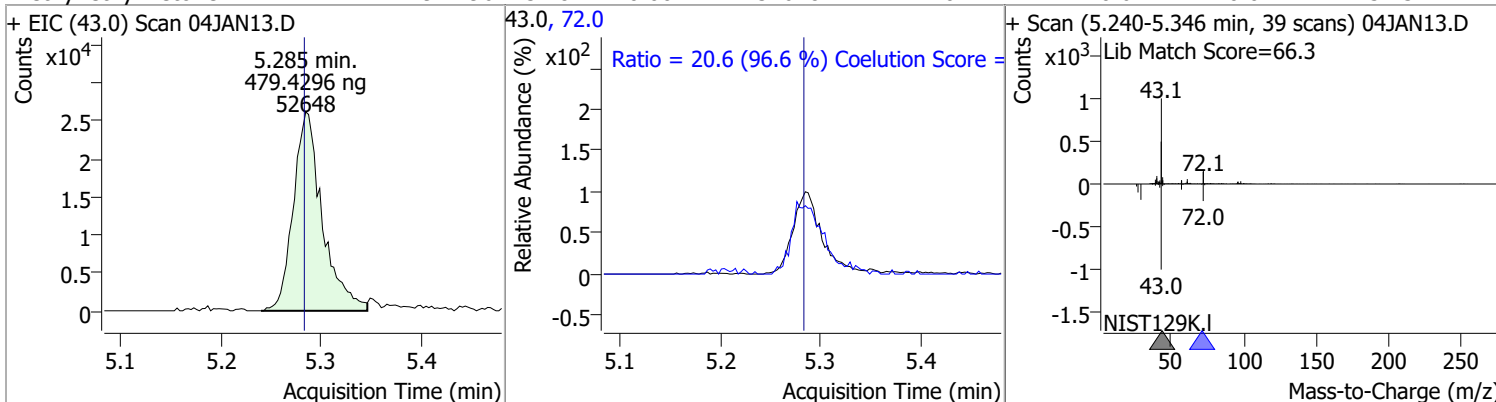


| Compound           | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|---------|------|----------|-------|------|--------|-------|-------|
| Bromochloromethane | 51.6233 | 5.52 | 0.00     | 17338 | 49.0 | 176.8  | 152.9 | 212.9 |

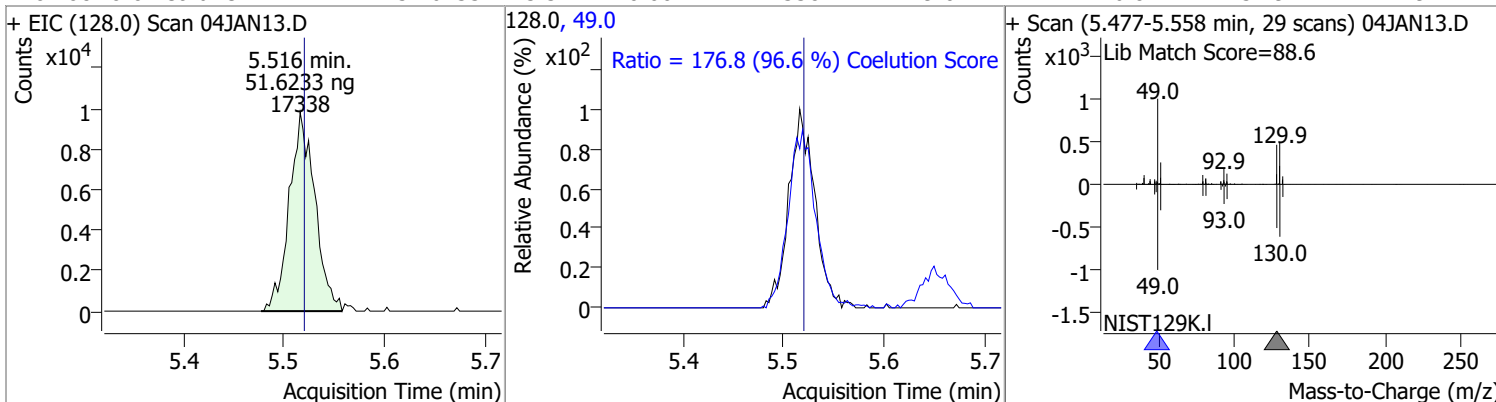


# Quantitation Results Report (QT Reviewed)


| Compound   | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|---------|------|----------|-------|------|--------|-------|-------|
| Chloroform | 48.2031 | 5.65 | 0.00     | 71403 | 85.0 | 65.5   | 36.0  | 96.0  |




| Compound              | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|---------|------|----------|-------|------|--------|-------|-------|
| 1,1,1-Trichloroethane | 48.2688 | 5.83 | 0.00     | 67007 | 99.0 | 65.2   | 34.7  | 94.7  |
|                       |         |      |          |       | 61.0 | 50.6   | 18.1  | 78.1  |



| Compound             | Conc.   | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|----------------------|---------|------|----------|-------|-------|--------|-------|-------|
| Dibromofluoromethane | 48.1661 | 5.85 | 0.00     | 35309 | 191.5 | 22.5   | 0.0   | 53.1  |




| Compound             | Conc.   | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|----------------------|---------|------|----------|-------|-------|--------|-------|-------|
| Carbon tetrachloride | 47.7520 | 6.03 | 0.00     | 65313 | 119.0 | 97.9   | 67.2  | 127.2 |
|                      |         |      |          |       | 121.0 | 32.5   | 0.1   | 60.1  |




# Quantitation Results Report (QT Reviewed)


| Compound            | Conc.   | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|---------------------|---------|------|----------|-------|-------|--------|-------|-------|
| 1,1-Dichloropropene | 47.7627 | 6.03 | 0.00     | 56376 | 110.0 | 35.3   | 5.9   | 65.9  |
|                     |         |      |          |       | 77.0  | 31.1   | 0.1   | 60.1  |

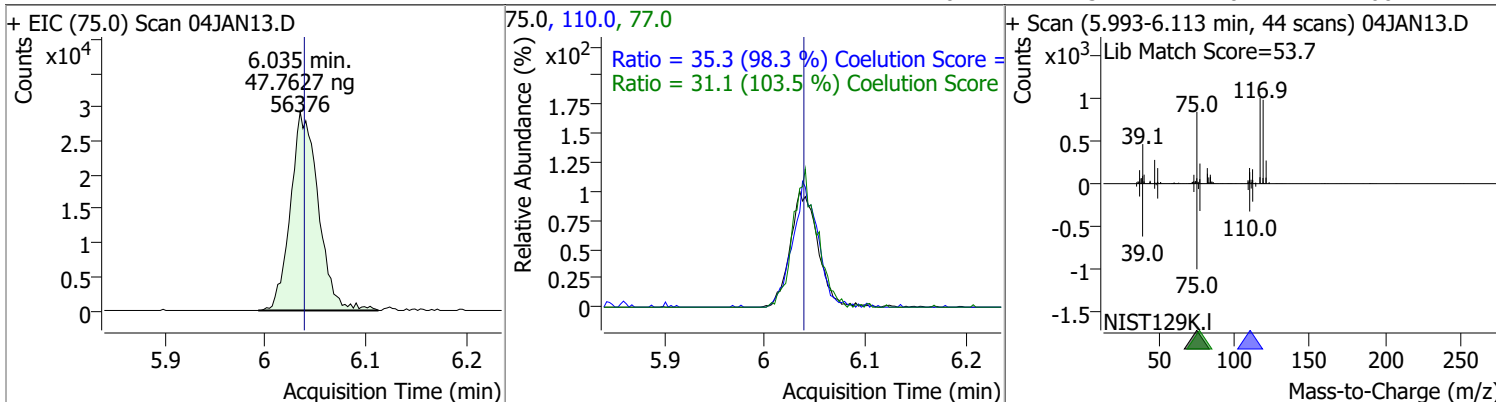


| Compound              | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|---------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 48.1252 | 6.23 | 0.00     | 15238 | 65.0 | 202.3  | 166.5 | 226.5 |

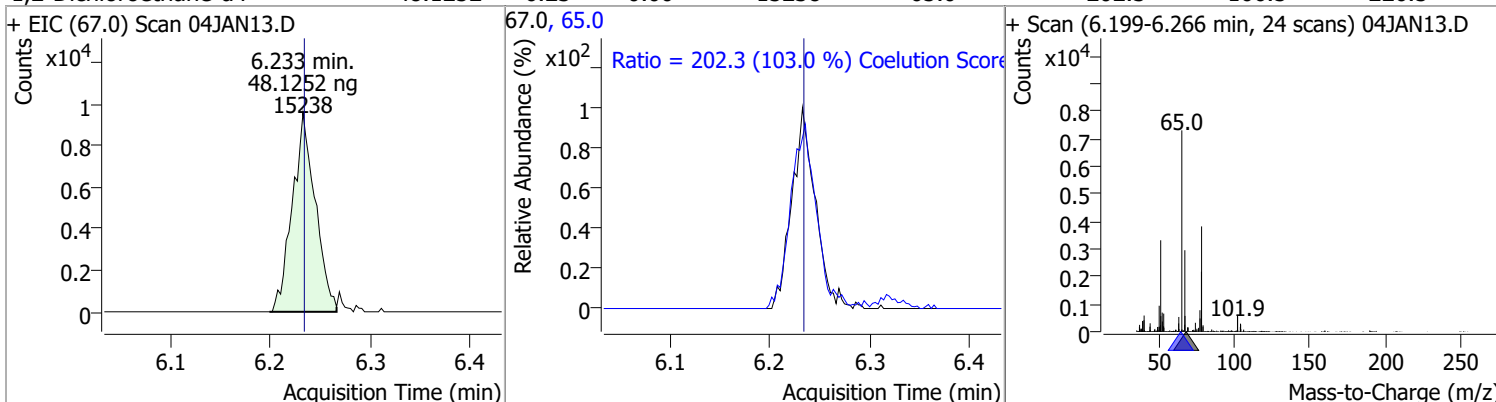

| Compound | Conc.   | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|----------|---------|------|----------|--------|------|--------|-------|-------|
| Benzene  | 48.0054 | 6.28 | 0.00     | 148727 | 77.0 | 23.7   | 0.0   | 53.5  |

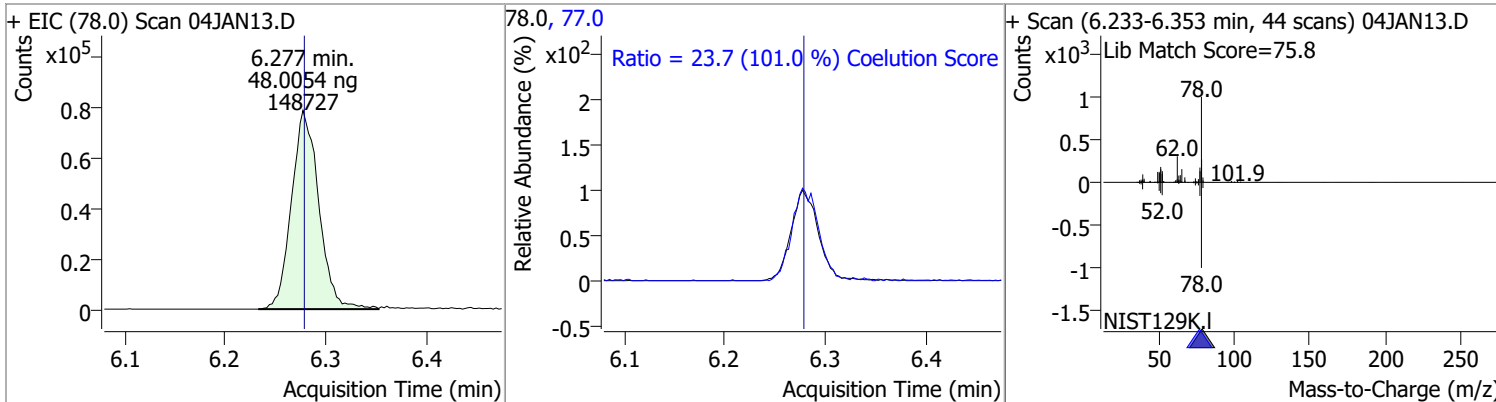


| Compound           | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|---------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane | 48.9880 | 6.32 | 0.00     | 41058 | 64.0 | 30.9   | 0.0   | 59.9  |
|                    |         |      |          |       | 98.0 | 5.5    | 0.0   | 37.6  |

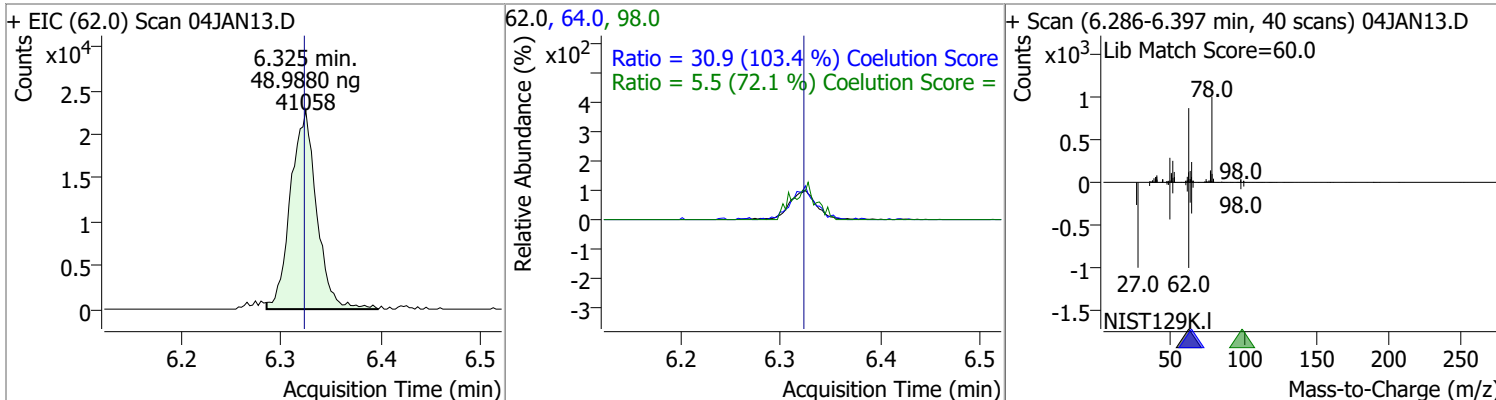


# Quantitation Results Report (QT Reviewed)


| Compound        | Conc.   | RT   | Dev(Min) | Resp. | QIon          | QRatio        | Lower        | Upper         |
|-----------------|---------|------|----------|-------|---------------|---------------|--------------|---------------|
| Trichloroethene | 47.1189 | 7.03 | 0.00     | 42682 | 130.0<br>97.0 | 102.4<br>66.2 | 71.5<br>34.1 | 131.5<br>94.1 |



| Compound            | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|---------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloropropane | 47.5273 | 7.27 | 0.00     | 37870 | 76.0 | 40.8   | 8.2   | 68.2  |

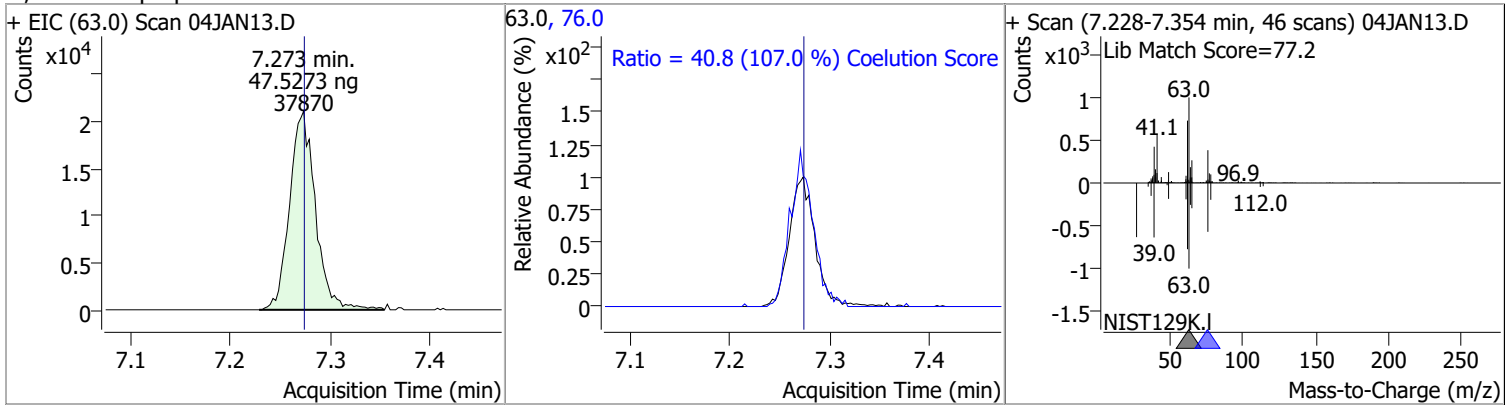


| Compound       | Conc.   | RT   | Dev(Min) | Resp. | QIon          | QRatio        | Lower        | Upper          |
|----------------|---------|------|----------|-------|---------------|---------------|--------------|----------------|
| Dibromomethane | 47.4844 | 7.40 | 0.00     | 15989 | 173.5<br>95.0 | 117.0<br>85.2 | 83.7<br>52.2 | 143.7<br>112.2 |

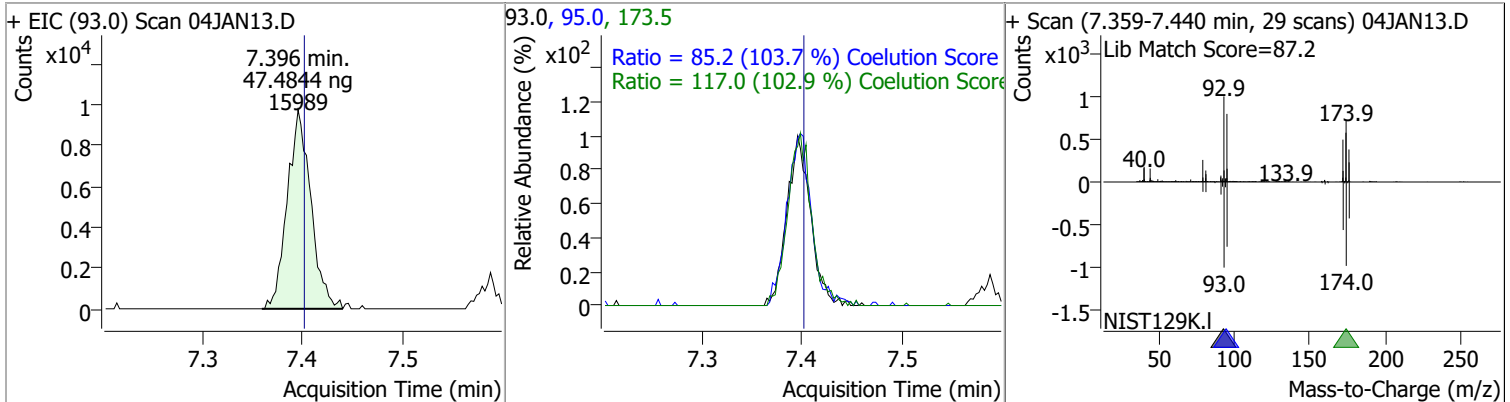


# Quantitation Results Report (QT Reviewed)


| Compound             | Conc.   | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|----------------------|---------|------|----------|-------|-------|--------|-------|-------|
| Bromodichloromethane | 47.2409 | 7.59 | 0.00     | 43900 | 85.0  | 67.1   | 34.5  | 94.5  |
|                      |         |      |          |       | 127.0 | 10.1   | 0.0   | 39.6  |



| Compound                | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------------------|---------|------|----------|-------|------|--------|-------|-------|
| cis-1,3-Dichloropropene | 46.5283 | 8.06 | 0.00     | 48886 | 39.0 | 56.3   | 23.3  | 83.3  |
|                         |         |      |          |       | 77.0 | 30.9   | 1.0   | 61.0  |




| Compound   | Conc.   | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|------------|---------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 47.1441 | 8.32 | 0.00     | 136453 | 100.0 | 63.8   | 34.4  | 94.4  |
|            |         |      |          |        | 99.0  | 9.2    | 0.0   | 39.6  |




# Quantitation Results Report (QT Reviewed)


| Compound | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|---------|------|----------|-------|------|--------|-------|-------|
| Toluene  | 47.0116 | 8.39 | 0.00     | 91915 | 91.0 | 175.7  | 145.8 | 205.8 |



| Compound                  | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|---------|------|----------|-------|------|--------|-------|-------|
| trans-1,3-Dichloropropene | 47.0378 | 8.64 | 0.00     | 35179 | 39.0 | 53.4   | 23.4  | 83.4  |
|                           |         |      |          |       | 77.0 | 32.7   | 2.4   | 62.4  |

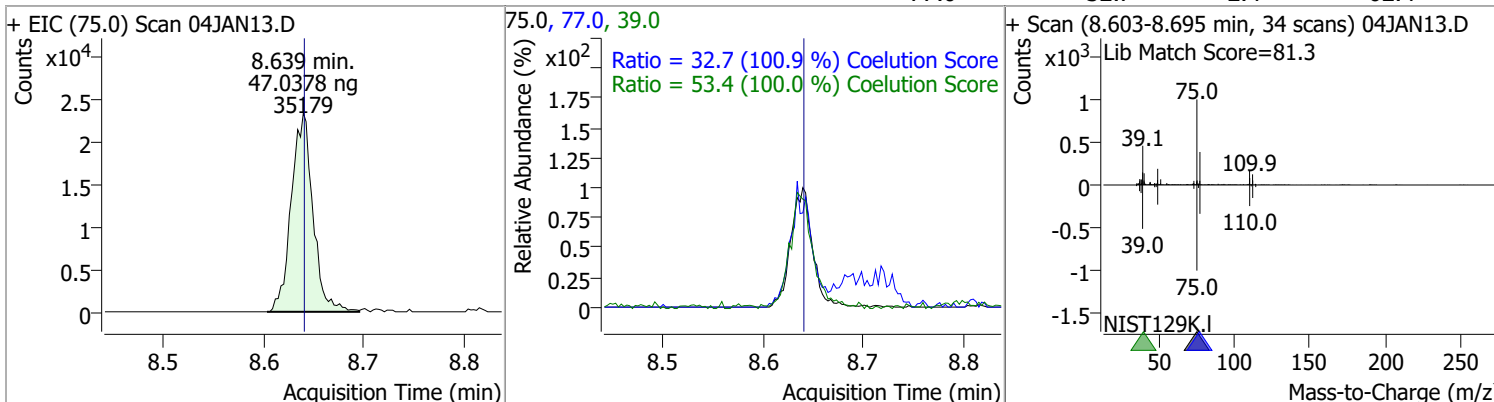


| Compound              | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|---------|------|----------|-------|------|--------|-------|-------|
| 1,1,2-Trichloroethane | 48.4759 | 8.82 | 0.00     | 18884 | 97.0 | 115.3  | 84.6  | 144.6 |
|                       |         |      |          |       | 85.0 | 65.7   | 37.6  | 97.6  |

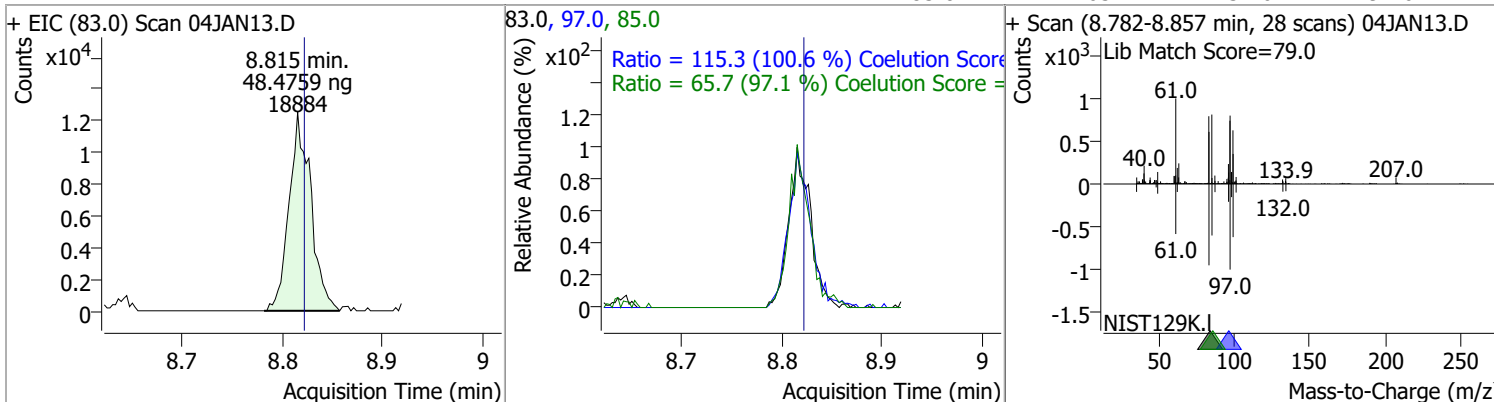


# Quantitation Results Report (QT Reviewed)


| Compound          | Conc.   | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|-------------------|---------|------|----------|-------|-------|--------|-------|-------|
| Tetrachloroethene | 46.2932 | 8.94 | 0.00     | 36925 | 165.8 | 132.7  | 98.6  | 158.6 |
|                   |         |      |          |       | 129.0 | 94.5   | 61.5  | 121.5 |




| Compound            | Conc.   | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|---------|------|----------|-------|------|--------|-------|-------|
| 1,3-Dichloropropane | 48.8841 | 8.98 | 0.00     | 37457 | 78.0 | 31.5   | 2.9   | 62.9  |







| Compound             | Conc.   | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|----------------------|---------|------|----------|-------|-------|--------|-------|-------|
| Chlorodibromomethane | 46.2411 | 9.20 | 0.00     | 28153 | 127.0 | 77.4   | 48.0  | 108.0 |



| Compound          | Conc.   | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|-------------------|---------|------|----------|-------|-------|--------|-------|-------|
| 1,2-Dibromoethane | 49.3889 | 9.30 | 0.00     | 21037 | 109.0 | 88.2   | 64.5  | 124.5 |




# Quantitation Results Report (QT Reviewed)

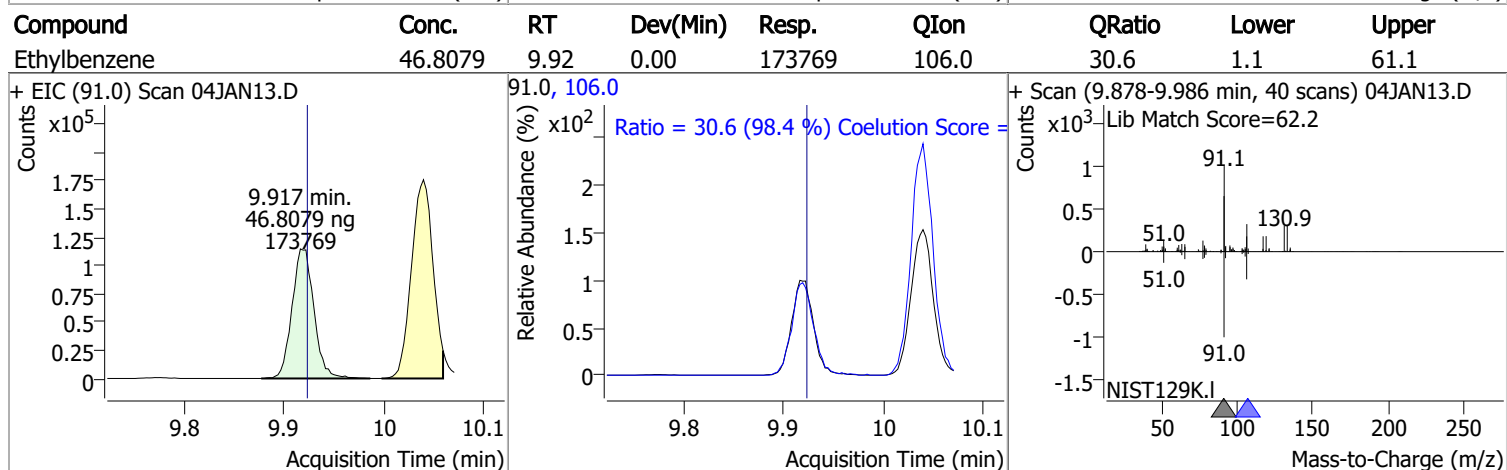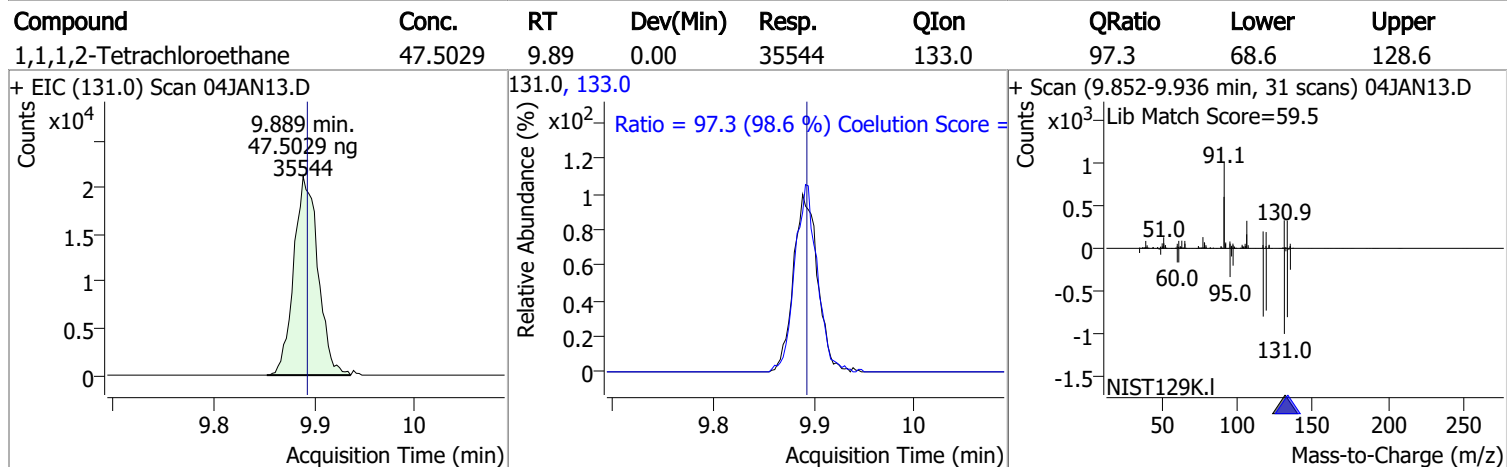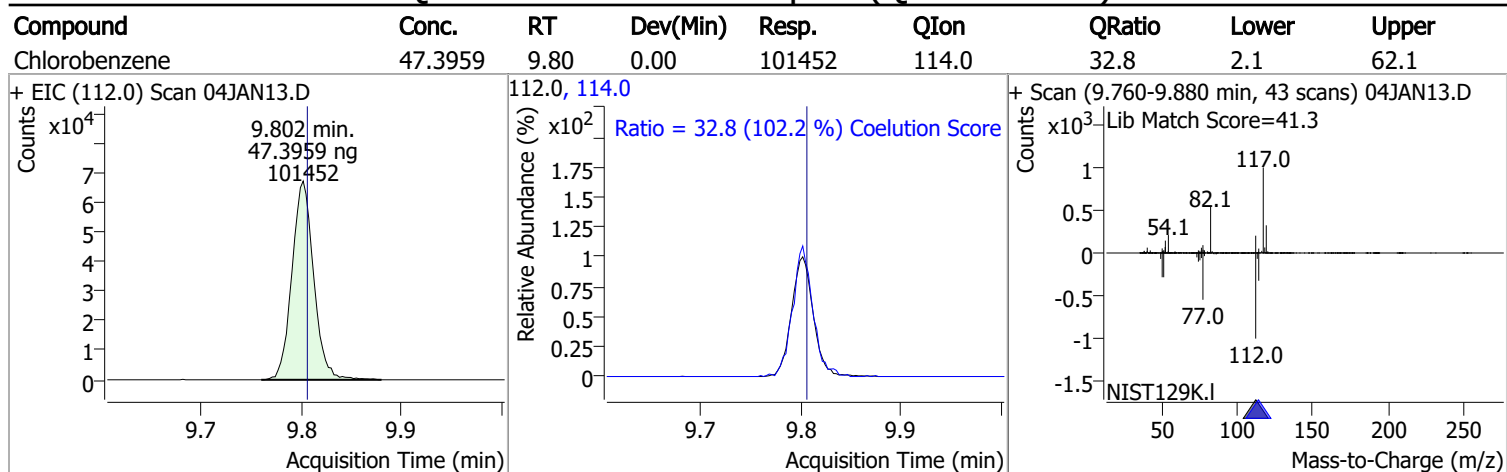




# Quantitation Results Report (QT Reviewed)


| Compound | Conc.   | RT    | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|---------|-------|----------|-------|------|--------|-------|-------|
| o-Xylene | 47.5086 | 10.43 | 0.00     | 61016 | 91.0 | 215.7  | 183.1 | 243.1 |

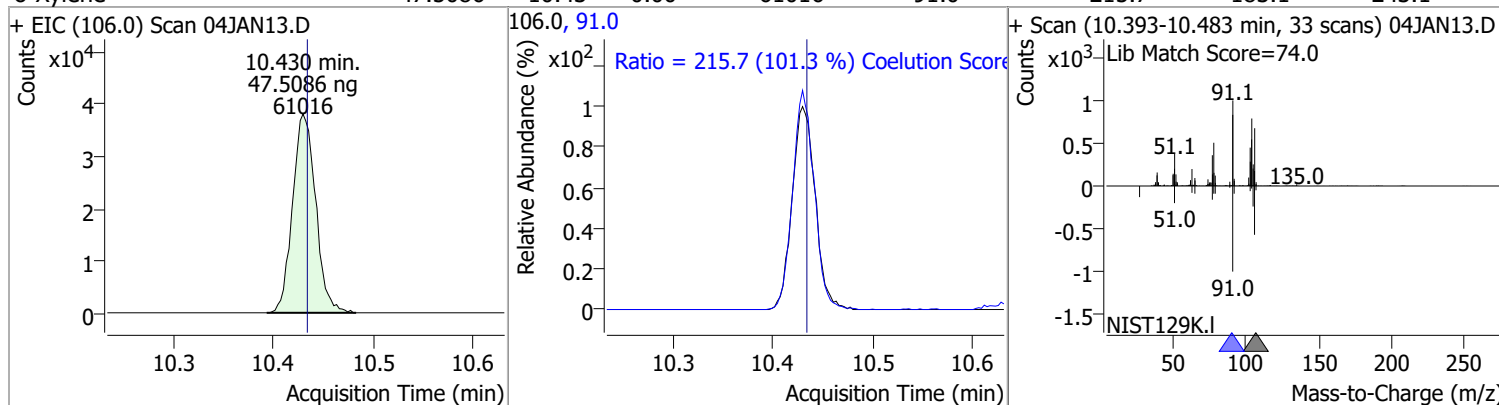


| Compound | Conc.   | RT    | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|---------|-------|----------|-------|------|--------|-------|-------|
| Styrene  | 46.7052 | 10.44 | 0.00     | 96576 | 78.0 | 49.7   | 19.6  | 79.6  |



| Compound  | Conc.   | RT    | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|-----------|---------|-------|----------|-------|-------|--------|-------|-------|
| Bromoform | 50.5170 | 10.62 | 0.00     | 16073 | 170.5 | 48.4   | 22.1  | 82.1  |
|           |         |       |          |       | 174.5 | 47.8   | 20.1  | 80.1  |




| Compound             | Conc.   | RT    | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|----------------------|---------|-------|----------|-------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 46.6647 | 10.95 | 0.00     | 42506 | 174.0 | 97.8   | 61.7  | 121.7 |
|                      |         |       |          |       | 176.0 | 93.2   | 60.6  | 120.6 |




# Quantitation Results Report (QT Reviewed)


| Compound     | Conc.   | RT    | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|--------------|---------|-------|----------|-------|-------|--------|-------|-------|
| Bromobenzene | 47.5759 | 11.09 | 0.00     | 38282 | 77.0  | 145.8  | 115.7 | 175.7 |
|              |         |       |          |       | 158.0 | 102.1  | 66.5  | 126.5 |




| Compound                  | Conc.   | RT    | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|---------|-------|----------|-------|------|--------|-------|-------|
| 1,1,2,2-Tetrachloroethane | 48.6124 | 11.10 | -0.01    | 22514 | 85.0 | 65.6   | 36.2  | 96.2  |

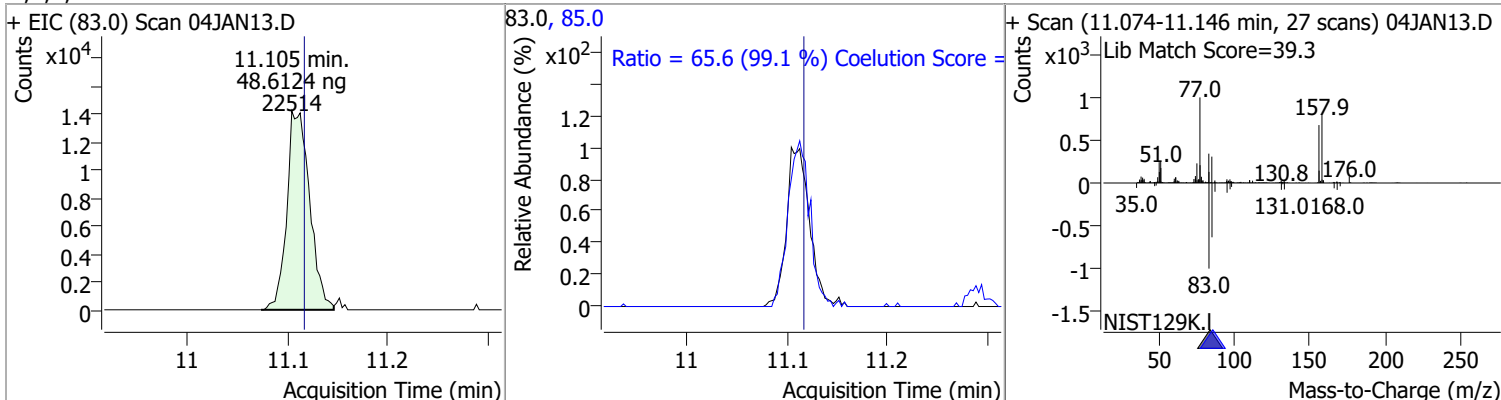

| Compound               | Conc.   | RT    | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|------------------------|---------|-------|----------|-------|-------|--------|-------|-------|
| 1,2,3-Trichloropropane | 49.1924 | 11.15 | 0.00     | 6096  | 112.0 | 60.8   | 33.5  | 93.5  |






| Compound        | Conc.   | RT    | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------|---------|-------|----------|-------|------|--------|-------|-------|
| 2-Chlorotoluene | 47.4466 | 11.29 | 0.00     | 37987 | 91.0 | 284.4  | 252.3 | 312.3 |






# Quantitation Results Report (QT Reviewed)




| Compound        | Conc.   | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|-----------------|---------|-------|----------|--------|-------|--------|-------|-------|
| 4-Chlorotoluene | 48.3865 | 11.40 | 0.00     | 126308 | 126.0 | 31.6   | 1.7   | 61.7  |

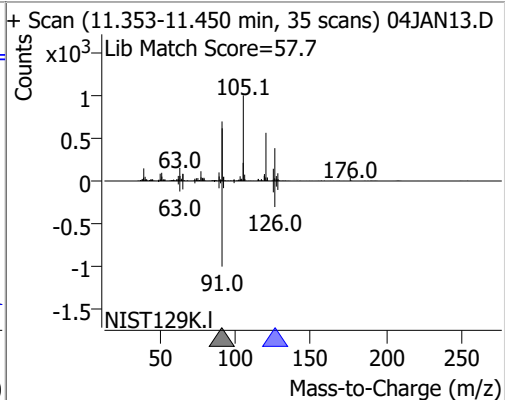

|                     |         |       |      |       |       |      |      |      |
|---------------------|---------|-------|------|-------|-------|------|------|------|
| 1,3-Dichlorobenzene | 47.3853 | 12.03 | 0.00 | 69539 | 148.0 | 63.6 | 33.6 | 93.6 |
|                     |         |       |      |       | 111.0 | 37.9 | 9.8  | 69.8 |

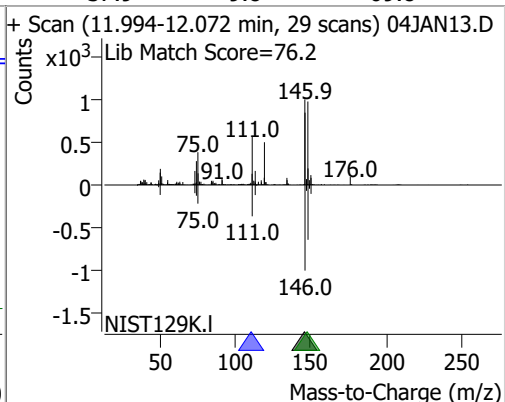




|                     |         |       |      |       |       |      |      |      |
|---------------------|---------|-------|------|-------|-------|------|------|------|
| 1,4-Dichlorobenzene | 48.0106 | 12.13 | 0.00 | 71841 | 148.0 | 64.5 | 33.1 | 93.1 |
|                     |         |       |      |       | 111.0 | 41.8 | 9.1  | 69.1 |

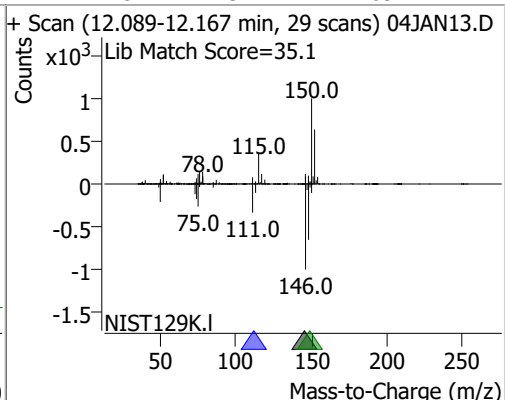


# Quantitation Results Report (QT Reviewed)

| Compound            | Conc.   | RT    | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|---------------------|---------|-------|----------|-------|-------|--------|-------|-------|
| 1,2-Dichlorobenzene | 48.5498 | 12.49 | 0.00     | 60213 | 148.0 | 61.9   | 33.9  | 93.9  |
|                     |         |       |          |       | 111.0 | 40.0   | 11.0  | 71.0  |

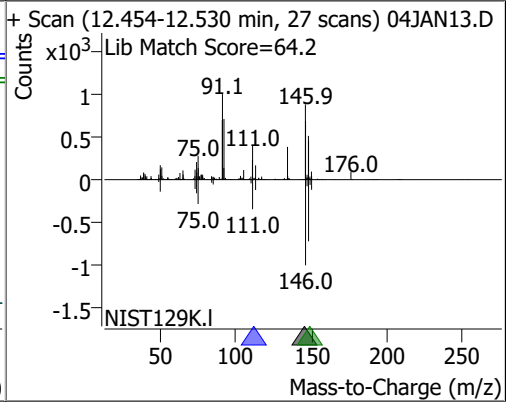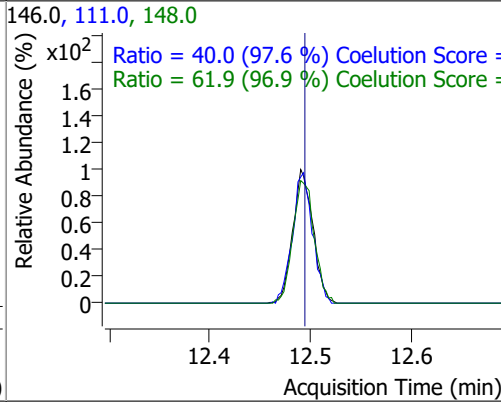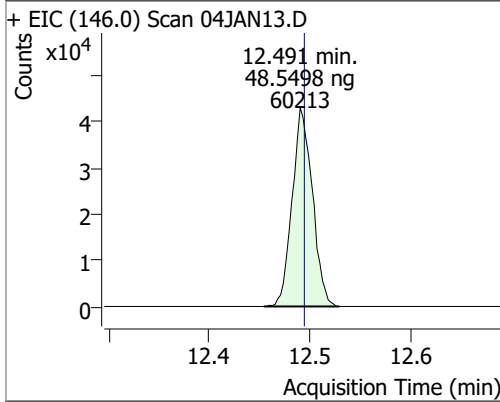

# Quantitation Results Report (QT Reviewed)

|                |                                     |                   |                       |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File      | 04JAN15.D                           | Operator          | MSC                   |
| Acq. Method    | 5975CACQF.M                         | Acq. Date-Time    | 1/4/2022 5:50:25 PM   |
| Sample Name    | ICAL010422_5                        | Instrument        | VOA5975C              |
| Vial           | 15                                  | Multiplier        | 1.00                  |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m  | Comment           |                       |
| Tune File      | BFB_Atune3.u                        | Tune Date         | 10/11/2021 4:02:00 PM |
| Batch Name     | VG010422_8260B.batch.bin            | Last Calib Update | 1/9/2022 8:59:52 PM   |
| Ref Library    | \\MASSHUNTER\Org\Library\NIST129K.I |                   |                       |



| Compound                           | RT                   | QIon  | Resp.  | Conc.             | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|-------------------|-------|----------|
| <b>Internal Standards</b>          |                      |       |        |                   |       |          |
| M Fluorobenzene                    | 6.623                | 96.0  | 823488 | 250.0000          | ng    | 0.000    |
| M Chlorobenzene-d5                 | 9.772                | 82.0  | 306491 | 250.0000          | ng    | 0.000    |
| M 1,4-Dichlorobenzene-d4           | 12.100               | 152.0 | 264477 | 250.0000          | ng    | 0.000    |
| <b>System Monitoring Compounds</b> |                      |       |        |                   |       |          |
| S Dibromofluoromethane             | 5.845                | 113.0 | 89307  | 115.1146          | ng    | 0.000    |
| Spiked Amount: 250.000             | Range: 80.0 - 119.0% |       |        | Recovery = 46.05% | *     |          |
| S 1,2-Dichloroethane-d4            | 6.233                | 67.0  | 39086  | 116.6420          | ng    | 0.000    |
| Spiked Amount: 250.000             | Range: 81.0 - 118.0% |       |        | Recovery = 46.66% | *     |          |
| S Toluene-d8                       | 8.319                | 98.0  | 358186 | 121.2749          | ng    | 0.000    |
| Spiked Amount: 250.000             | Range: 89.0 - 112.0% |       |        | Recovery = 48.51% | *     |          |
| S p-Bromofluorobenzene             | 10.954               | 95.0  | 114269 | 117.9350          | ng    | 0.000    |
| Spiked Amount: 250.000             | Range: 85.0 - 114.0% |       |        | Recovery = 47.17% | *     |          |
| <b>Target Compounds</b>            |                      |       |        |                   |       |          |
| T Dichlorodifluoromethane          | 1.241                | 85.0  | 137933 | 127.8193          | ng    | 100      |
| T Chloromethane                    | 1.409                | 50.0  | 160604 | 122.6179          | ng    | 100      |
| T Vinyl chloride                   | 1.495                | 62.0  | 148358 | 125.8809          | ng    | 100      |
| T Bromomethane                     | 1.799                | 96.0  | 65163  | 123.6504          | ng    | 100      |
| T Chloroethane                     | 1.894                | 64.0  | 71420  | 122.4086          | ng    | 100      |
| T Trichlorofluoromethane           | 2.142                | 101.0 | 188808 | 129.0687          | ng    | 100      |
| T 1,1-Dichloroethene               | 2.697                | 96.0  | 99438  | 119.8798          | ng    | 100      |
| T Methylene chloride               | 3.336                | 49.0  | 135271 | 110.6249          | ng    | 100      |
| T trans-1,2-Dichloroethene         | 3.718                | 96.0  | 100409 | 118.6511          | ng    | 100      |
| T Methyl tert-butyl ether (MTBE)   | 3.754                | 73.0  | 139068 | 127.1375          | ng    | 100      |
| T 1,1-Dichloroethane               | 4.378                | 63.0  | 186052 | 118.1125          | ng    | 100      |
| T 2,2-Dichloropropane              | 5.196                | 77.0  | 139656 | 118.3203          | ng    | 100      |
| T cis-1,2-Dichloroethene           | 5.215                | 96.0  | 100057 | 116.6190          | ng    | 100      |
| T Methyl ethyl ketone              | 5.282                | 43.0  | 134730 | 1159.3019         | ng    | 100      |
| T Bromochloromethane               | 5.519                | 128.0 | 41966  | 118.0683          | ng    | 100      |
| T Chloroform                       | 5.653                | 83.0  | 179640 | 114.5912          | ng    | 100      |


# Quantitation Results Report (QT Reviewed)

| Compound                    | RT     | QIon  | Resp.  | Conc.    | Units | Dev(Min) |
|-----------------------------|--------|-------|--------|----------|-------|----------|
| T 1,1,1-Trichloroethane     | 5.834  | 97.0  | 174206 | 118.5764 | ng    | 100      |
| T Carbon tetrachloride      | 6.024  | 117.0 | 172928 | 119.4667 | ng    | 100      |
| T 1,1-Dichloropropene       | 6.038  | 75.0  | 149649 | 119.8002 | ng    | 100      |
| T Benzene                   | 6.278  | 78.0  | 383469 | 116.9553 | ng    | 100      |
| T 1,2-Dichloroethane        | 6.322  | 62.0  | 104855 | 118.2143 | ng    | 100      |
| T Trichloroethene           | 7.030  | 95.0  | 114123 | 123.4646 | ng    | 100      |
| T 1,2-Dichloropropane       | 7.270  | 63.0  | 99187  | 121.9890 | ng    | 100      |
| T Dibromomethane            | 7.399  | 93.0  | 40628  | 118.2425 | ng    | 100      |
| T Bromodichloromethane      | 7.585  | 83.0  | 115664 | 121.9749 | ng    | 100      |
| T cis-1,3-Dichloropropene   | 8.059  | 75.0  | 129419 | 120.7116 | ng    | 100      |
| T Toluene                   | 8.389  | 92.0  | 244712 | 122.6571 | ng    | 100      |
| T trans-1,3-Dichloropropene | 8.637  | 75.0  | 92719  | 121.4929 | ng    | 100      |
| T 1,1,2-Trichloroethane     | 8.818  | 83.0  | 46673  | 117.4130 | ng    | 100      |
| T Tetrachloroethene         | 8.935  | 163.8 | 97590  | 119.9003 | ng    | 100      |
| T 1,3-Dichloropropane       | 8.980  | 76.0  | 96183  | 123.0132 | ng    | 100      |
| T Chlorodibromomethane      | 9.206  | 129.0 | 75015  | 120.7454 | ng    | 100      |
| T 1,2-Dibromoethane         | 9.306  | 107.0 | 51827  | 119.2394 | ng    | 100      |
| T Chlorobenzene             | 9.802  | 112.0 | 263617 | 120.6903 | ng    | 100      |
| T 1,1,1,2-Tetrachloroethane | 9.889  | 131.0 | 90898  | 119.0492 | ng    | 100      |
| T Ethylbenzene              | 9.920  | 91.0  | 464148 | 122.5243 | ng    | 100      |
| T m+p-Xylenes               | 10.039 | 106.0 | 368418 | 250.2587 | ng    | 100      |
| T o-Xylene                  | 10.430 | 106.0 | 161509 | 123.2378 | ng    | 100      |
| T Styrene                   | 10.447 | 104.0 | 268375 | 127.1910 | ng    | 100      |
| T Bromoform                 | 10.628 | 172.5 | 39165  | 115.7218 | ng    | 100      |
| T Bromobenzene              | 11.094 | 156.0 | 102265 | 119.4801 | ng    | 100      |
| T 1,1,2,2-Tetrachloroethane | 11.116 | 83.0  | 56958  | 115.6179 | ng    | 100      |
| T 1,2,3-Trichloropropane    | 11.147 | 110.0 | 14846  | 112.6261 | ng    | 100      |
| T 2-Chlorotoluene           | 11.292 | 126.0 | 102424 | 120.2675 | ng    | 100      |
| T 4-Chlorotoluene           | 11.400 | 91.0  | 336146 | 121.0591 | ng    | 100      |
| T 1,3-Dichlorobenzene       | 12.031 | 146.0 | 183404 | 117.4899 | ng    | 100      |
| T 1,4-Dichlorobenzene       | 12.125 | 146.0 | 189045 | 118.7699 | ng    | 100      |
| T 1,2-Dichlorobenzene       | 12.493 | 146.0 | 152284 | 115.4323 | ng    | 100      |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (\*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

# Quantitation Results Report (QT Reviewed)


| Compound                | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|-------------------------|----------|------|----------|--------|------|--------|-------|-------|
| Dichlorodifluoromethane | 127.8193 | 1.24 | 0.00     | 137933 | 87.0 | 32.3   | 2.3   | 62.3  |




| Compound      | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------|----------|------|----------|--------|------|--------|-------|-------|
| Chloromethane | 122.6179 | 1.41 | 0.00     | 160604 | 52.0 | 32.1   | 2.1   | 62.1  |



| Compound       | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|----------------|----------|------|----------|--------|------|--------|-------|-------|
| Vinyl chloride | 125.8809 | 1.50 | 0.00     | 148358 | 64.0 | 29.9   | 0.0   | 59.9  |




| Compound     | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|----------|------|----------|-------|------|--------|-------|-------|
| Bromomethane | 123.6504 | 1.80 | 0.00     | 65163 | 94.0 | 104.6  | 74.6  | 134.6 |




# Quantitation Results Report (QT Reviewed)


| Compound     | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|----------|------|----------|-------|------|--------|-------|-------|
| Chloroethane | 122.4086 | 1.89 | 0.00     | 71420 | 66.0 | 30.1   | 0.1   | 60.1  |

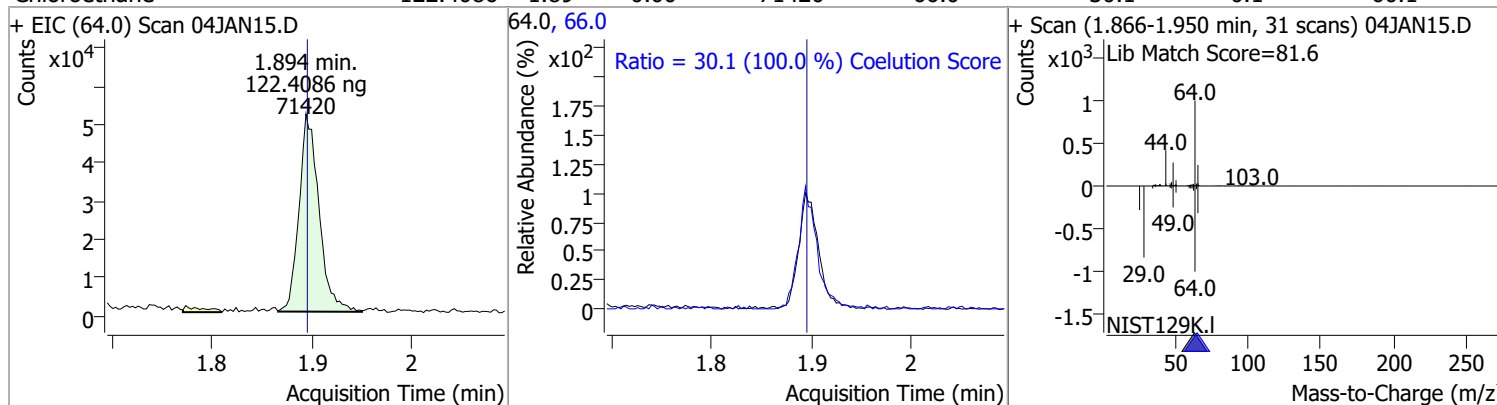


| Compound               | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|------------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Trichlorofluoromethane | 129.0687 | 2.14 | 0.00     | 188808 | 103.0 | 64.2   | 34.2  | 94.2  |

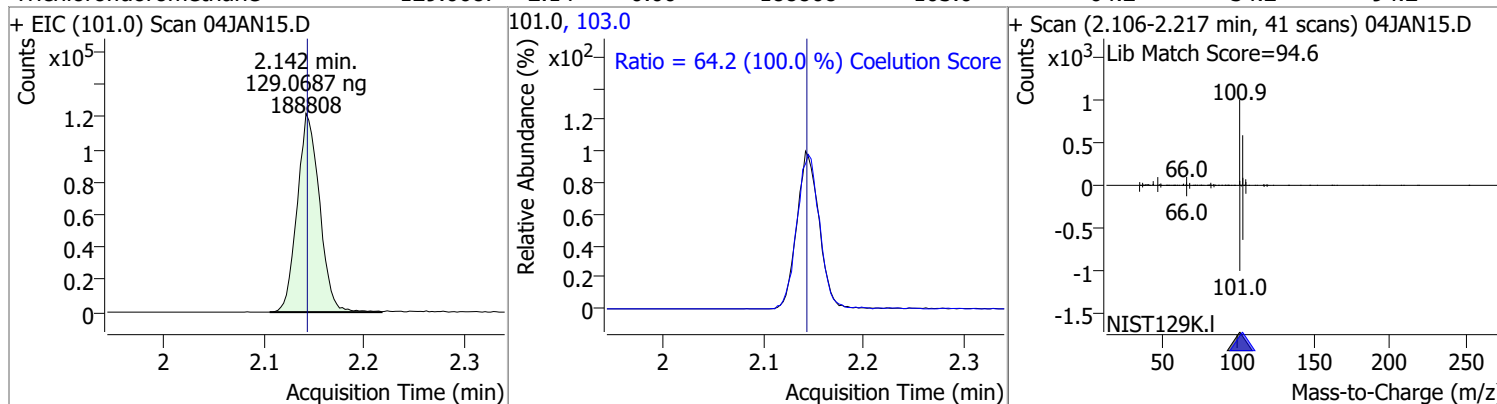

| Compound           | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,1-Dichloroethene | 119.8798 | 2.70 | 0.00     | 99438 | 61.0 | 180.3  | 150.3 | 210.3 |
|                    |          |      |          |       | 63.0 | 56.7   | 26.7  | 86.7  |

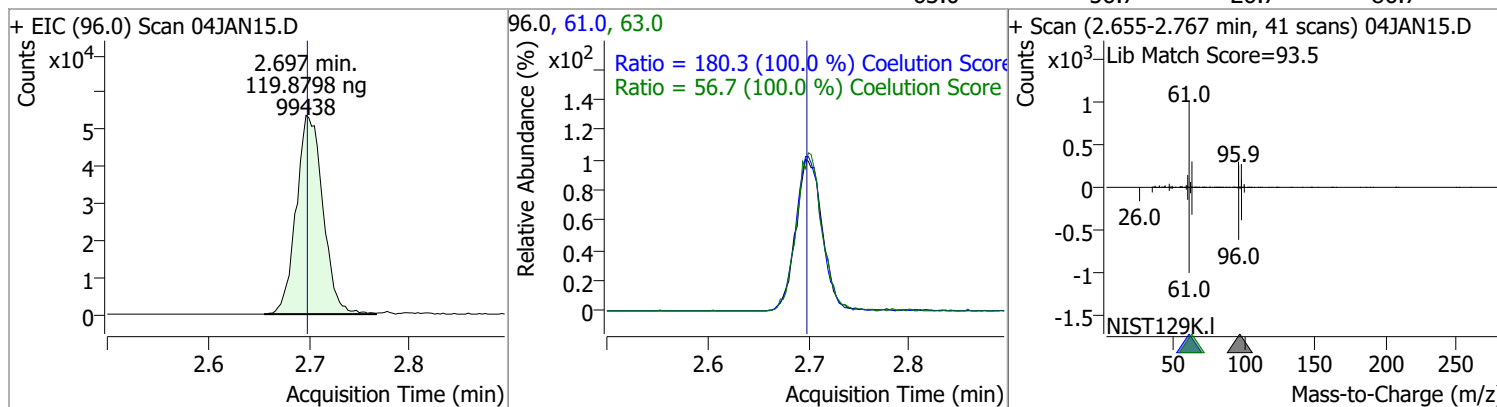


| Compound           | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| Methylene chloride | 110.6249 | 3.34 | 0.00     | 135271 | 84.0 | 66.9   | 36.9  | 96.9  |
|                    |          |      |          |        | 86.0 | 44.3   | 14.3  | 74.3  |

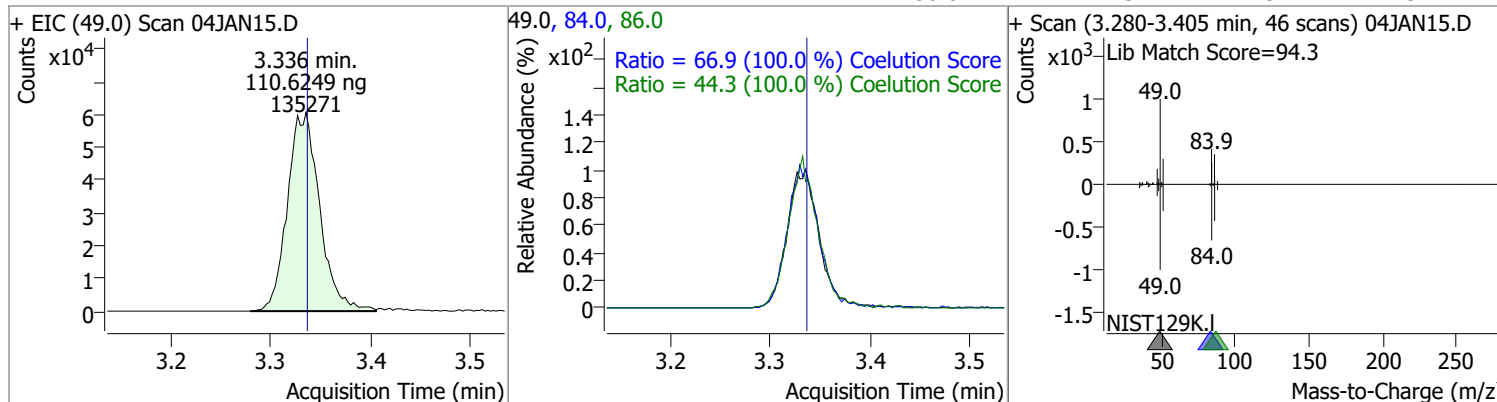




# Quantitation Results Report (QT Reviewed)


| Compound                 | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------------|----------|------|----------|--------|------|--------|-------|-------|
| trans-1,2-Dichloroethene | 118.6511 | 3.72 | 0.00     | 100409 | 61.0 | 153.9  | 123.9 | 183.9 |
|                          |          |      |          |        | 98.0 | 65.7   | 35.7  | 95.7  |



| Compound                       | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------------------|----------|------|----------|--------|------|--------|-------|-------|
| Methyl tert-butyl ether (MTBE) | 127.1375 | 3.75 | 0.00     | 139068 | 57.0 | 24.6   | 0.0   | 54.6  |




| Compound           | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1-Dichloroethane | 118.1125 | 4.38 | 0.00     | 186052 | 65.0 | 32.1   | 2.1   | 62.1  |
|                    |          |      |          |        | 83.0 | 13.7   | 0.0   | 43.7  |




# Quantitation Results Report (QT Reviewed)


| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 2,2-Dichloropropane | 118.3203 | 5.20 | 0.00     | 139656 | 41.0 | 66.5   | 36.5  | 96.5  |
|                     |          |      |          |        | 97.0 | 23.2   | 0.0   | 53.2  |




| Compound               | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,2-Dichloroethene | 116.6190 | 5.22 | 0.00     | 100057 | 61.0 | 167.2  | 137.2 | 197.2 |
|                        |          |      |          |        | 98.0 | 67.3   | 37.3  | 97.3  |



| Compound            | Conc.     | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|-----------|------|----------|--------|------|--------|-------|-------|
| Methyl ethyl ketone | 1159.3019 | 5.28 | 0.00     | 134730 | 72.0 | 21.3   | 0.0   | 51.3  |




| Compound           | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|-------|------|--------|-------|-------|
| Bromochloromethane | 118.0683 | 5.52 | 0.00     | 41966 | 49.0 | 182.9  | 152.9 | 212.9 |




# Quantitation Results Report (QT Reviewed)


| Compound   | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|------|--------|-------|-------|
| Chloroform | 114.5912 | 5.65 | 0.00     | 179640 | 85.0 | 66.0   | 36.0  | 96.0  |




| Compound              | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1,1-Trichloroethane | 118.5764 | 5.83 | 0.00     | 174206 | 99.0 | 64.7   | 34.7  | 94.7  |
|                       |          |      |          |        | 61.0 | 48.1   | 18.1  | 78.1  |



| Compound             | Conc.    | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|----------------------|----------|------|----------|-------|-------|--------|-------|-------|
| Dibromofluoromethane | 115.1146 | 5.85 | 0.00     | 89307 | 191.5 | 23.1   | 0.0   | 53.1  |




| Compound             | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Carbon tetrachloride | 119.4667 | 6.02 | 0.00     | 172928 | 119.0 | 97.2   | 67.2  | 127.2 |
|                      |          |      |          |        | 121.0 | 30.1   | 0.1   | 60.1  |




# Quantitation Results Report (QT Reviewed)


| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|-------|--------|-------|-------|
| 1,1-Dichloropropene | 119.8002 | 6.04 | 0.00     | 149649 | 110.0 | 35.9   | 5.9   | 65.9  |
|                     |          |      |          |        | 77.0  | 30.1   | 0.1   | 60.1  |

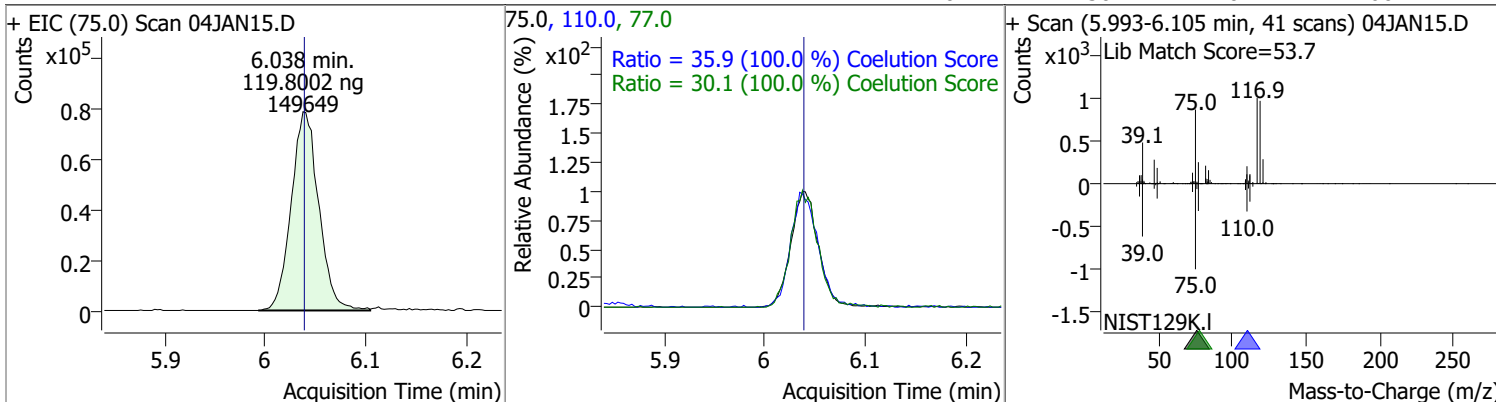


| Compound              | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 116.6420 | 6.23 | 0.00     | 39086 | 65.0 | 196.5  | 166.5 | 226.5 |

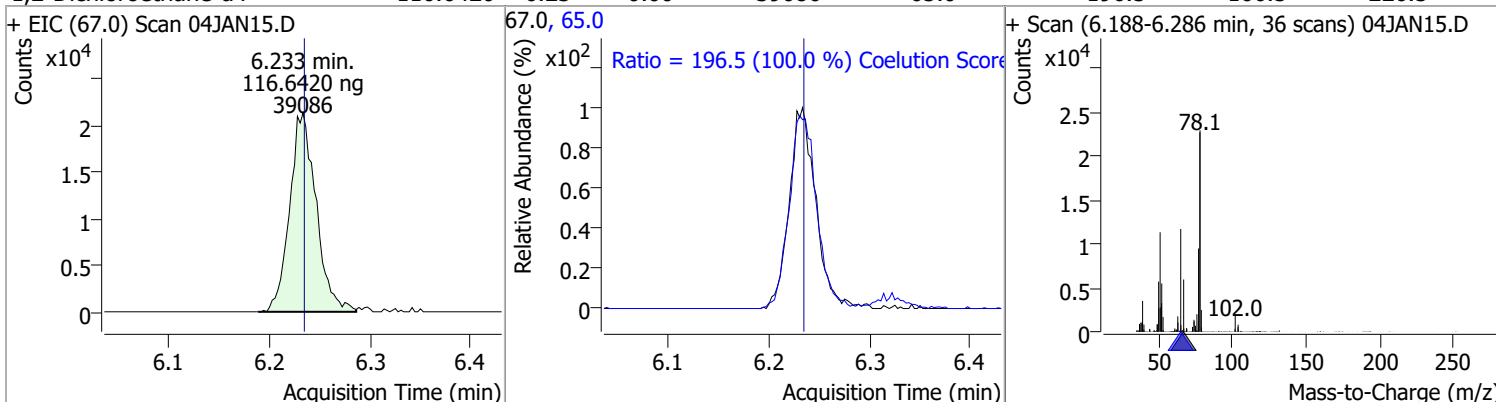

| Compound | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|----------|----------|------|----------|--------|------|--------|-------|-------|
| Benzene  | 116.9553 | 6.28 | 0.00     | 383469 | 77.0 | 23.5   | 0.0   | 53.5  |

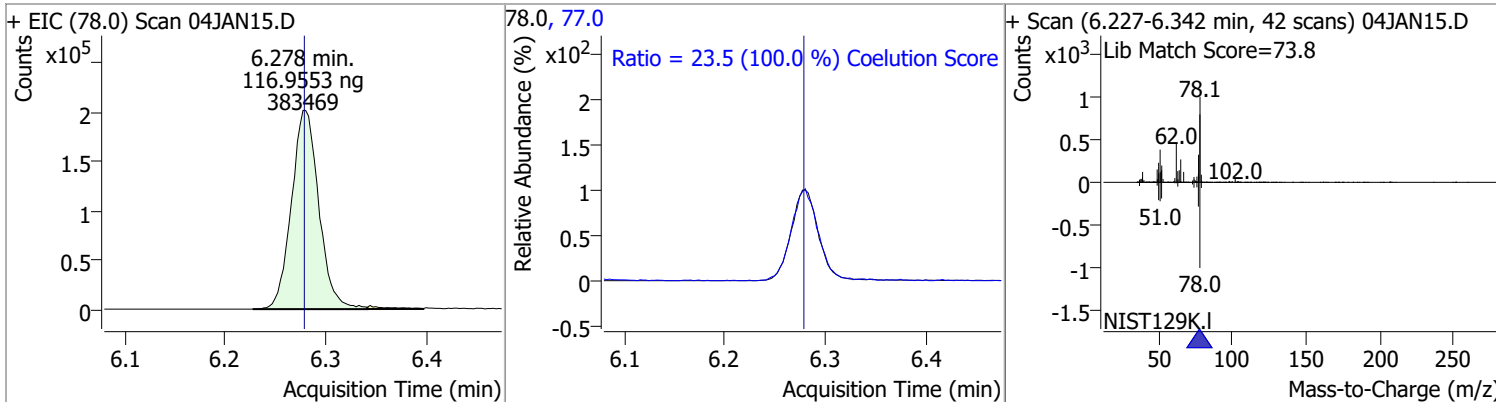


| Compound           | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloroethane | 118.2143 | 6.32 | 0.00     | 104855 | 64.0 | 29.9   | 0.0   | 59.9  |
|                    |          |      |          |        | 98.0 | 7.6    | 0.0   | 37.6  |




# Quantitation Results Report (QT Reviewed)


| Compound        | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|-----------------|----------|------|----------|--------|-------|--------|-------|-------|
| Trichloroethene | 123.4646 | 7.03 | 0.00     | 114123 | 130.0 | 101.5  | 71.5  | 131.5 |
|                 |          |      |          |        | 97.0  | 64.1   | 34.1  | 94.1  |

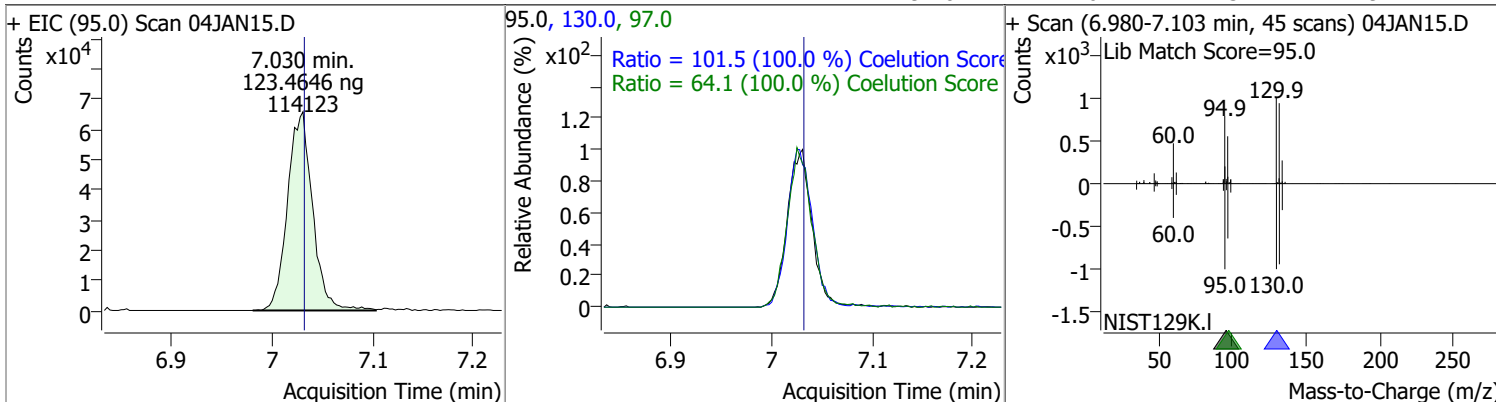

| Compound            | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloropropane | 121.9890 | 7.27 | 0.00     | 99187 | 76.0 | 38.2   | 8.2   | 68.2  |

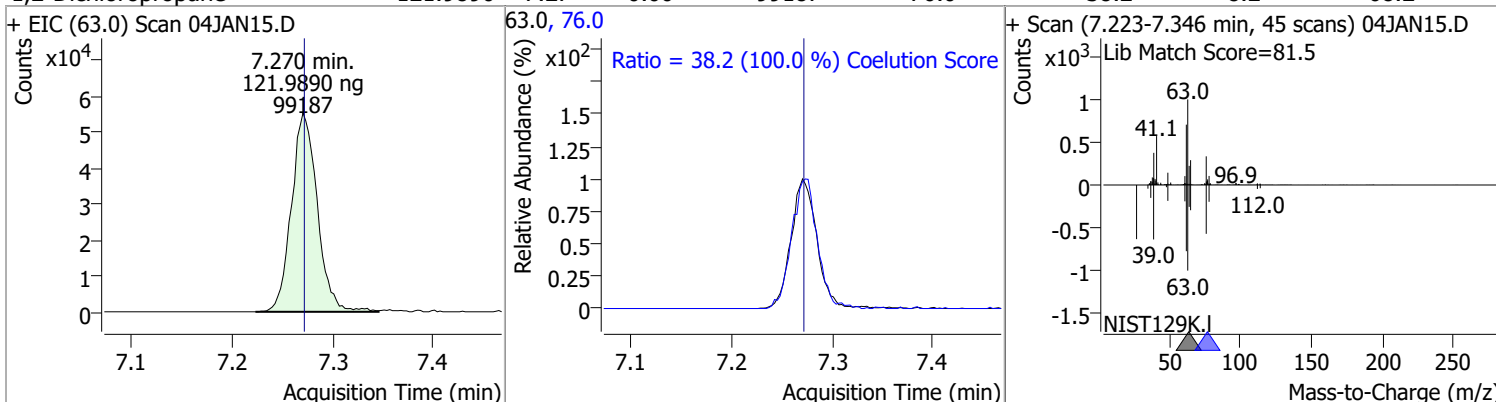


| Compound       | Conc.    | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|----------------|----------|------|----------|-------|-------|--------|-------|-------|
| Dibromomethane | 118.2425 | 7.40 | 0.00     | 40628 | 173.5 | 113.7  | 83.7  | 143.7 |
|                |          |      |          |       | 95.0  | 82.2   | 52.2  | 112.2 |

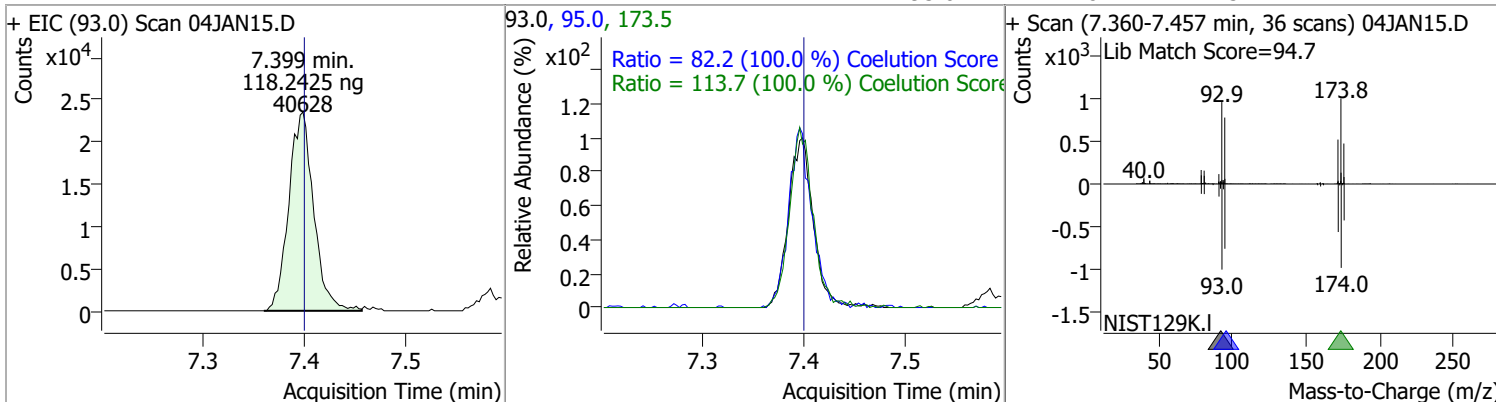


# Quantitation Results Report (QT Reviewed)


| Compound             | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Bromodichloromethane | 121.9749 | 7.59 | 0.00     | 115664 | 85.0  | 64.5   | 34.5  | 94.5  |
|                      |          |      |          |        | 127.0 | 9.6    | 0.0   | 39.6  |

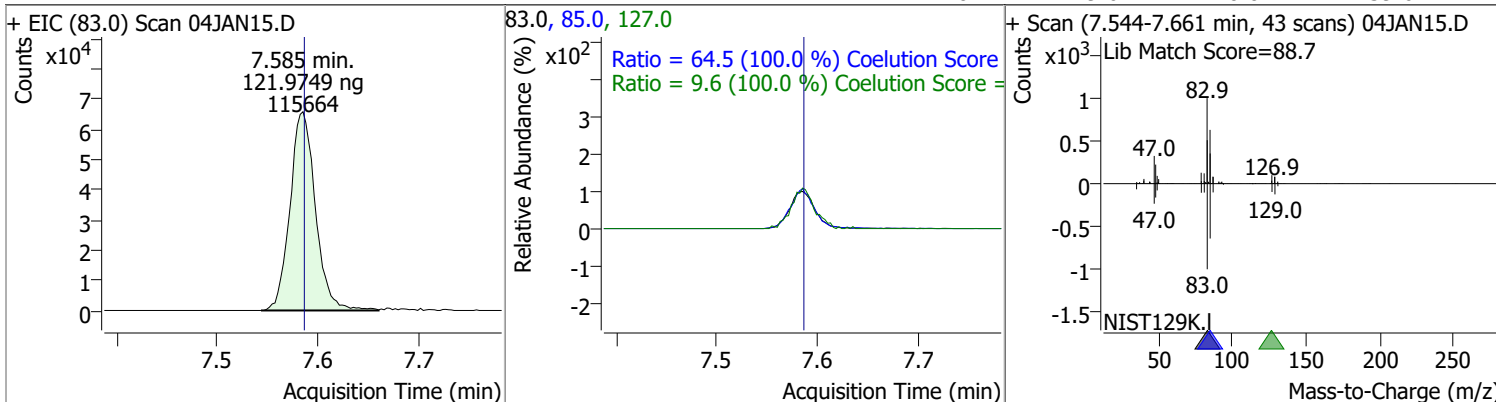

| Compound                | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|-------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,3-Dichloropropene | 120.7116 | 8.06 | 0.00     | 129419 | 39.0 | 53.3   | 23.3  | 83.3  |
|                         |          |      |          |        | 77.0 | 31.0   | 1.0   | 61.0  |

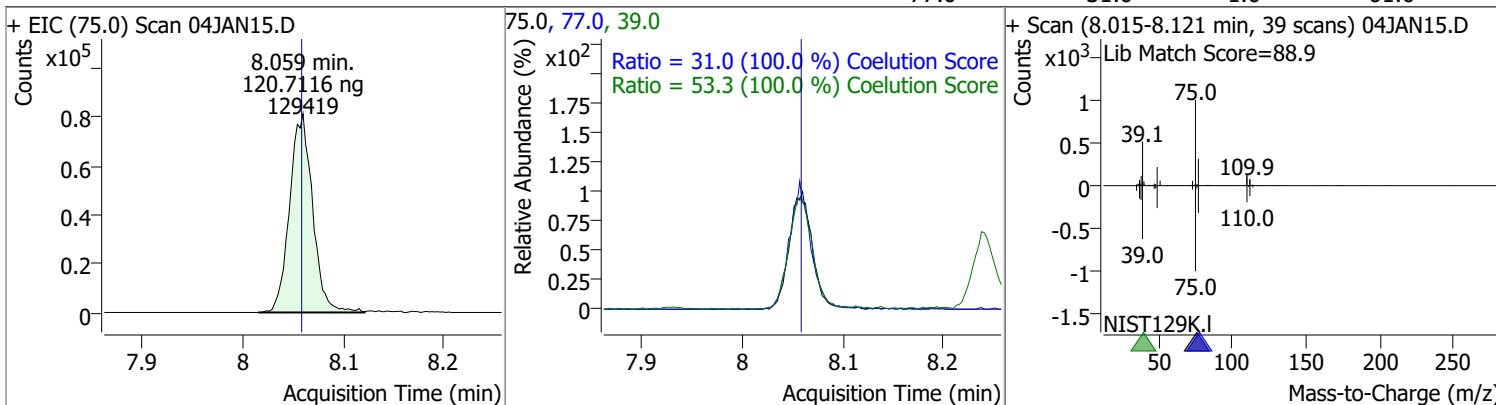


| Compound   | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 121.2749 | 8.32 | 0.00     | 358186 | 100.0 | 64.4   | 34.4  | 94.4  |
|            |          |      |          |        | 99.0  | 9.6    | 0.0   | 39.6  |

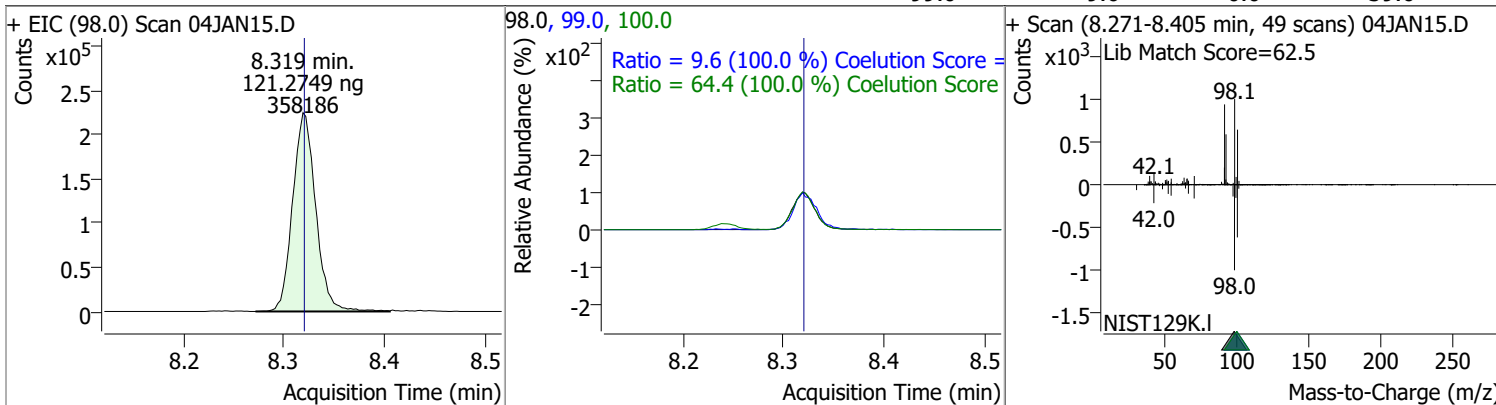


# Quantitation Results Report (QT Reviewed)


| Compound | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|----------|----------|------|----------|--------|------|--------|-------|-------|
| Toluene  | 122.6571 | 8.39 | 0.00     | 244712 | 91.0 | 175.8  | 145.8 | 205.8 |

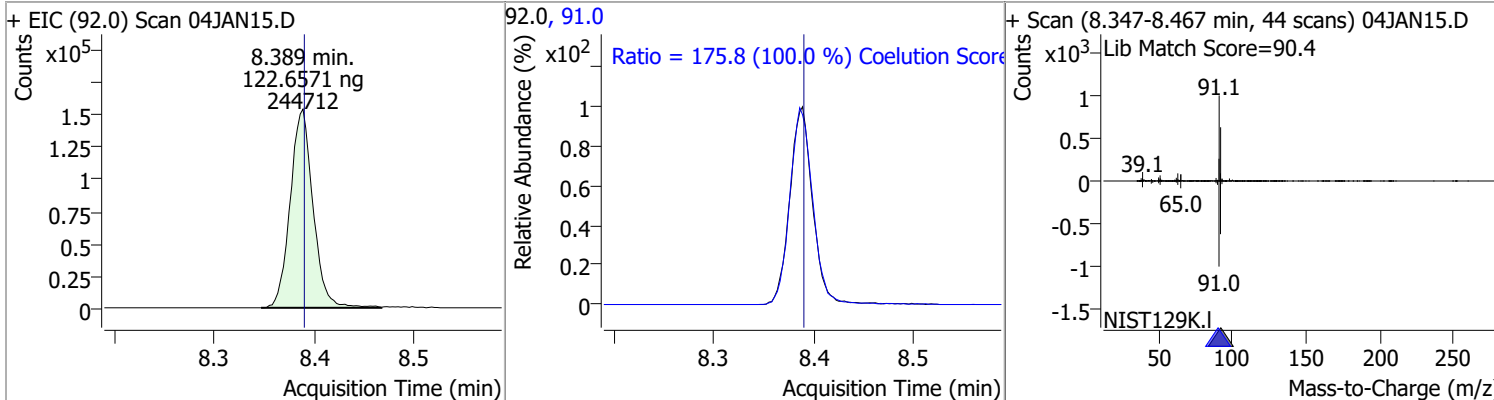

| Compound                  | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|----------|------|----------|-------|------|--------|-------|-------|
| trans-1,3-Dichloropropene | 121.4929 | 8.64 | 0.00     | 92719 | 39.0 | 53.4   | 23.4  | 83.4  |
|                           |          |      |          |       | 77.0 | 32.4   | 2.4   | 62.4  |

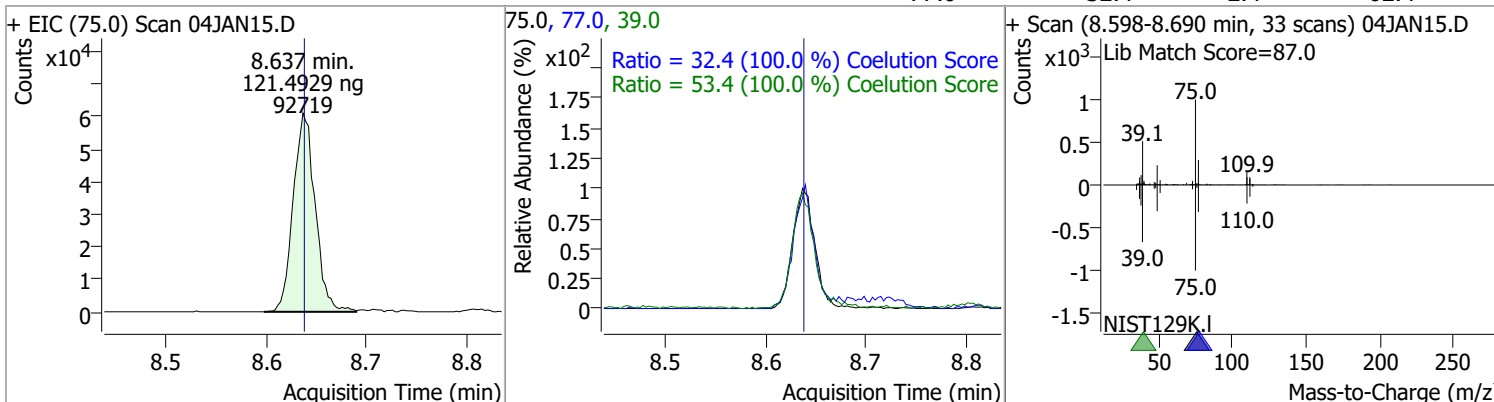

| Compound              | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,1,2-Trichloroethane | 117.4130 | 8.82 | 0.00     | 46673 | 97.0 | 114.6  | 84.6  | 144.6 |
|                       |          |      |          |       | 85.0 | 67.6   | 37.6  | 97.6  |

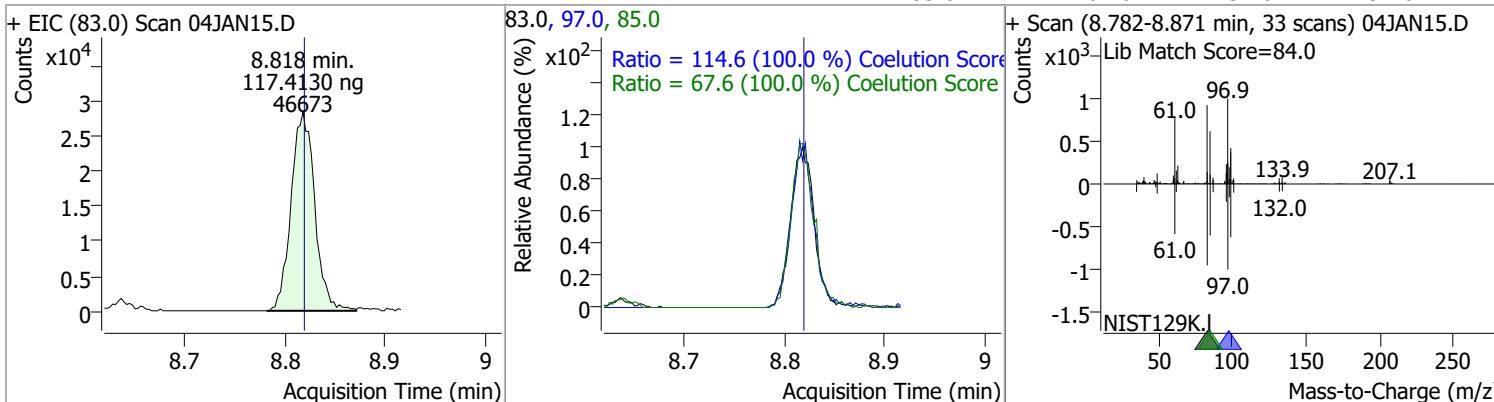


# Quantitation Results Report (QT Reviewed)

| Compound                     | Conc.    | RT                                                                                | Dev(Min)            | Resp. | QIon           | QRatio                                       | Lower        | Upper          |
|------------------------------|----------|-----------------------------------------------------------------------------------|---------------------|-------|----------------|----------------------------------------------|--------------|----------------|
| Tetrachloroethene            | 119.9003 | 8.94                                                                              | 0.00                | 97590 | 165.8<br>129.0 | 128.6<br>91.5                                | 98.6<br>61.5 | 158.6<br>121.5 |
| + EIC (163.8) Scan 04JAN15.D |          |                                                                                   | 163.8, 129.0, 165.8 |       |                | + Scan (8.896-8.999 min, 37 scans) 04JAN15.D |              |                |
|                              |          | Ratio = 91.5 (100.0 %) Coelution Score<br>Ratio = 128.6 (100.0 %) Coelution Score |                     |       |                |                                              |              |                |
| 1,3-Dichloropropane          | 123.0132 | 8.98                                                                              | 0.00                | 96183 | 78.0           | 32.9                                         | 2.9          | 62.9           |
| + EIC (76.0) Scan 04JAN15.D  |          |                                                                                   | 76.0, 78.0          |       |                | + Scan (8.938-9.036 min, 36 scans) 04JAN15.D |              |                |
|                              |          | Ratio = 32.9 (100.0 %) Coelution Score                                            |                     |       |                |                                              |              |                |
| Chlorodibromomethane         | 120.7454 | 9.21                                                                              | 0.00                | 75015 | 127.0          | 78.0                                         | 48.0         | 108.0          |
| + EIC (129.0) Scan 04JAN15.D |          |                                                                                   | 129.0, 127.0        |       |                | + Scan (9.164-9.264 min, 37 scans) 04JAN15.D |              |                |
|                              |          | Ratio = 78.0 (100.0 %) Coelution Score                                            |                     |       |                |                                              |              |                |
| 1,2-Dibromoethane            | 119.2394 | 9.31                                                                              | 0.00                | 51827 | 109.0          | 94.5                                         | 64.5         | 124.5          |
| + EIC (107.0) Scan 04JAN15.D |          |                                                                                   | 107.0, 109.0        |       |                | + Scan (9.264-9.370 min, 38 scans) 04JAN15.D |              |                |
|                              |          | Ratio = 94.5 (100.0 %) Coelution Score                                            |                     |       |                |                                              |              |                |




# Quantitation Results Report (QT Reviewed)


| Compound      | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|---------------|----------|------|----------|--------|-------|--------|-------|-------|
| Chlorobenzene | 120.6903 | 9.80 | 0.00     | 263617 | 114.0 | 32.1   | 2.1   | 62.1  |

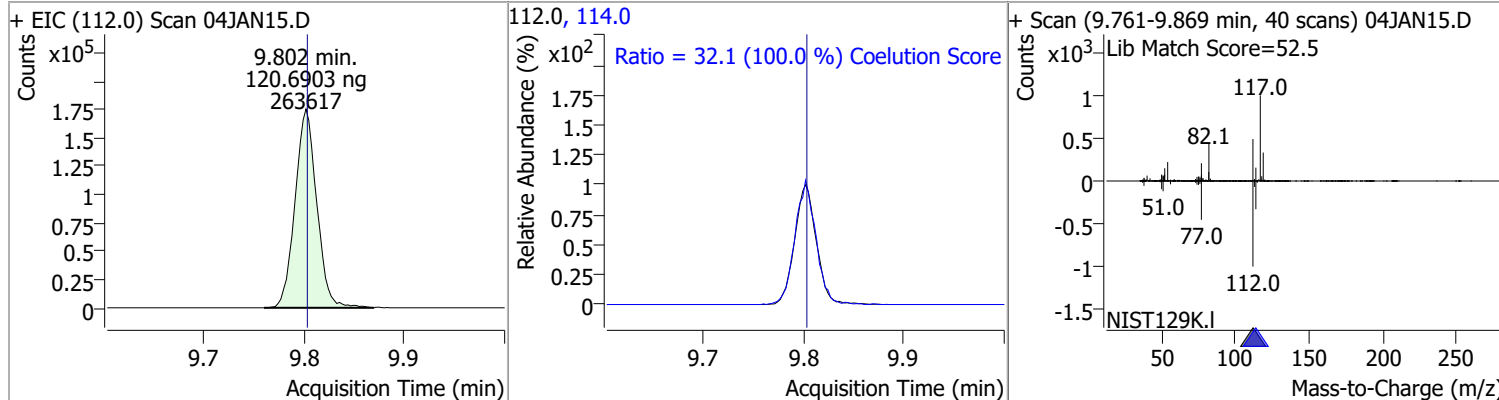


| Compound                  | Conc.    | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|---------------------------|----------|------|----------|-------|-------|--------|-------|-------|
| 1,1,1,2-Tetrachloroethane | 119.0492 | 9.89 | 0.00     | 90898 | 133.0 | 98.6   | 68.6  | 128.6 |

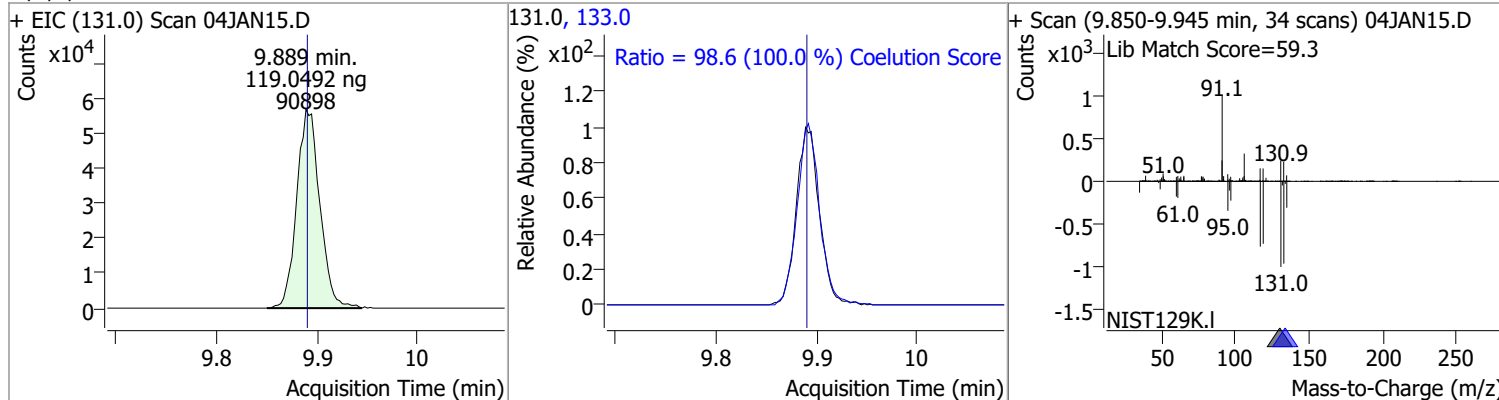

| Compound     | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|--------------|----------|------|----------|--------|-------|--------|-------|-------|
| Ethylbenzene | 122.5243 | 9.92 | 0.00     | 464148 | 106.0 | 31.1   | 1.1   | 61.1  |




| Compound    | Conc.    | RT    | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|-------------|----------|-------|----------|--------|------|--------|-------|-------|
| m+p-Xylenes | 250.2587 | 10.04 | 0.00     | 368418 | 91.0 | 201.4  | 171.4 | 231.4 |




# Quantitation Results Report (QT Reviewed)


| Compound | Conc.    | RT    | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|----------|----------|-------|----------|--------|------|--------|-------|-------|
| o-Xylene | 123.2378 | 10.43 | 0.00     | 161509 | 91.0 | 213.1  | 183.1 | 243.1 |

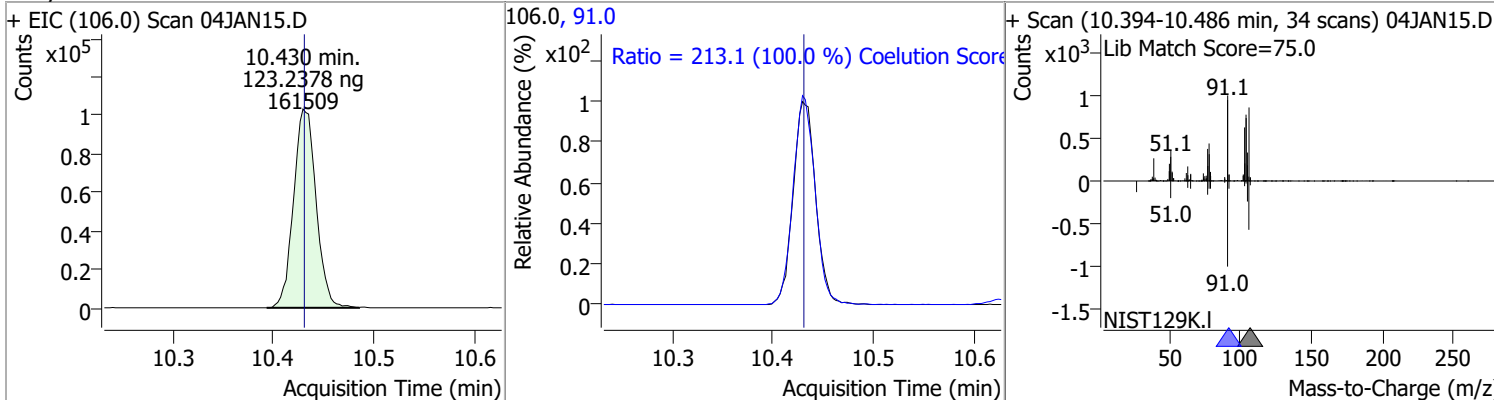


| Compound | Conc.    | RT    | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|----------|----------|-------|----------|--------|------|--------|-------|-------|
| Styrene  | 127.1910 | 10.45 | 0.00     | 268375 | 78.0 | 49.6   | 19.6  | 79.6  |

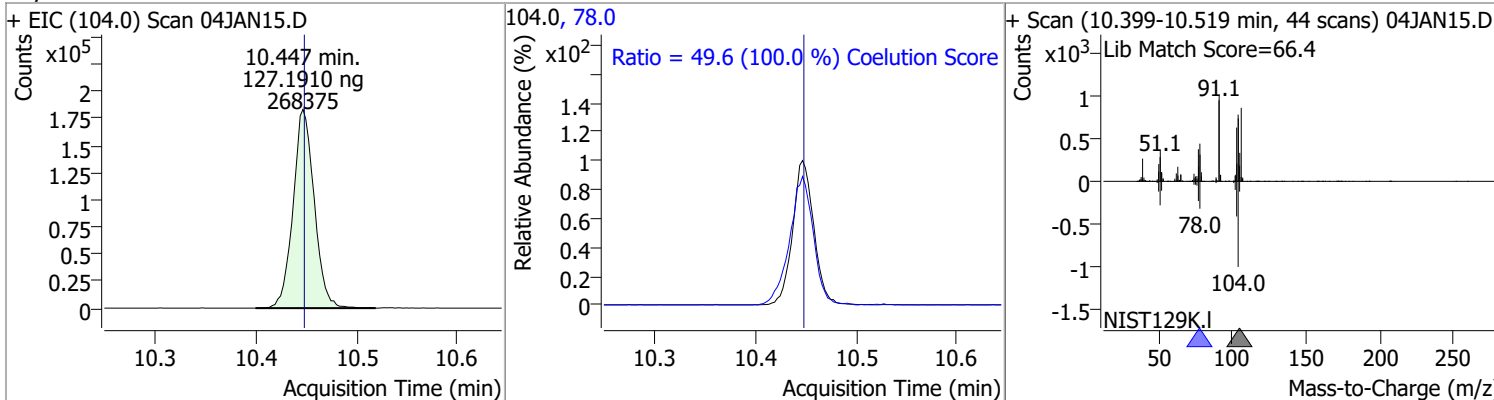

| Compound  | Conc.    | RT    | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|-----------|----------|-------|----------|-------|-------|--------|-------|-------|
| Bromoform | 115.7218 | 10.63 | 0.00     | 39165 | 170.5 | 52.1   | 22.1  | 82.1  |
|           |          |       |          |       | 174.5 | 50.1   | 20.1  | 80.1  |

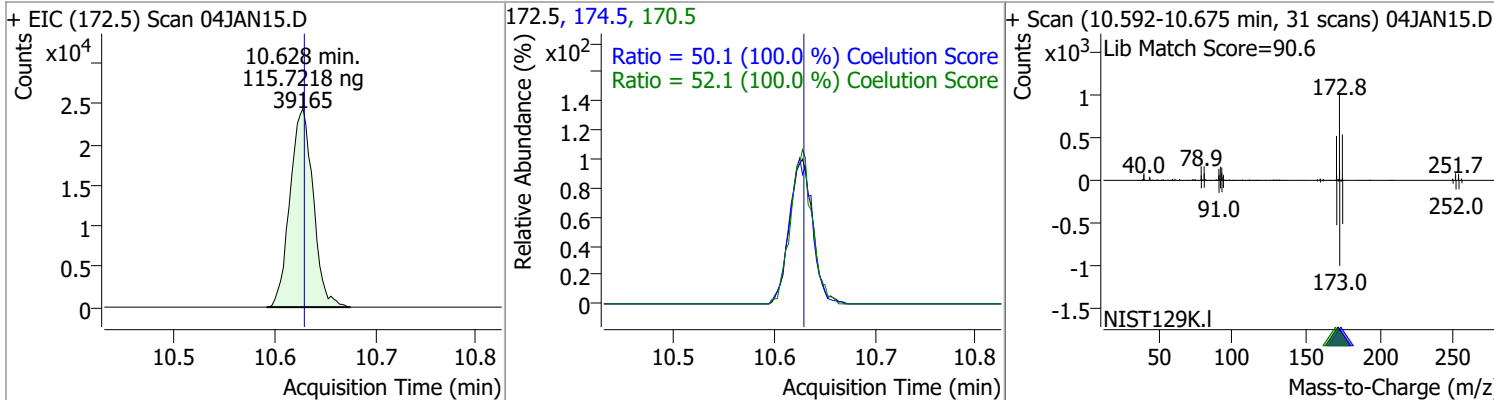


| Compound             | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 117.9350 | 10.95 | 0.00     | 114269 | 174.0 | 91.7   | 61.7  | 121.7 |
|                      |          |       |          |        | 176.0 | 90.6   | 60.6  | 120.6 |

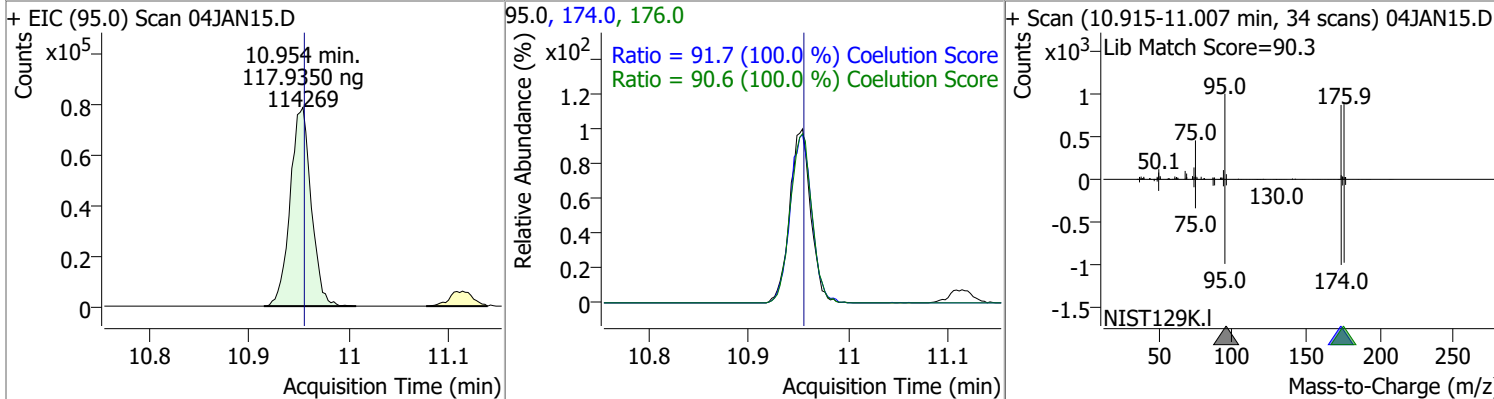


# Quantitation Results Report (QT Reviewed)


| Compound     | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|--------------|----------|-------|----------|--------|-------|--------|-------|-------|
| Bromobenzene | 119.4801 | 11.09 | 0.00     | 102265 | 77.0  | 145.7  | 115.7 | 175.7 |
|              |          |       |          |        | 158.0 | 96.5   | 66.5  | 126.5 |

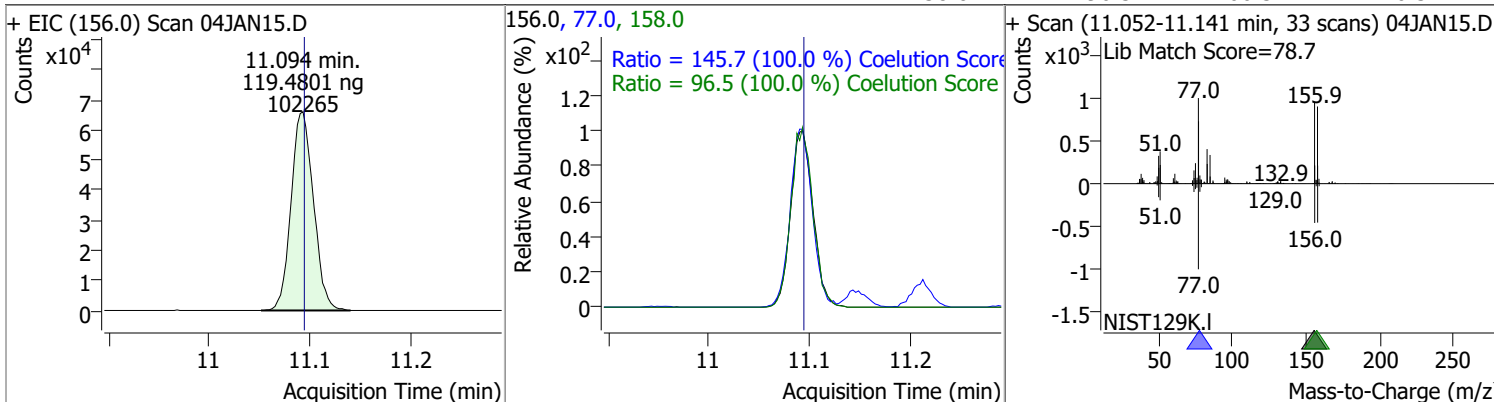


| Compound                  | Conc.    | RT    | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|----------|-------|----------|-------|------|--------|-------|-------|
| 1,1,2,2-Tetrachloroethane | 115.6179 | 11.12 | 0.00     | 56958 | 85.0 | 66.2   | 36.2  | 96.2  |

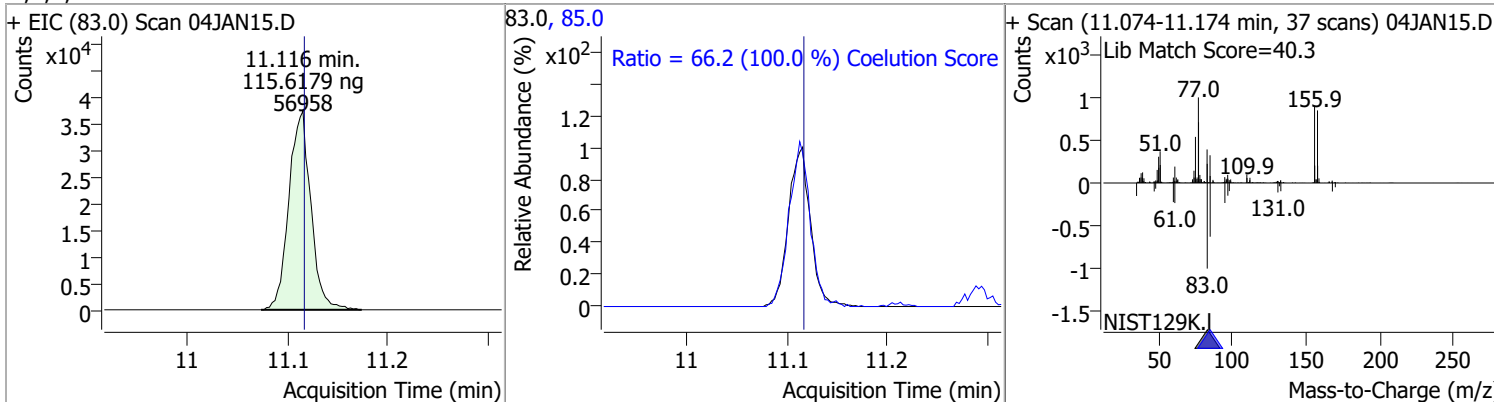

| Compound               | Conc.    | RT    | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|------------------------|----------|-------|----------|-------|-------|--------|-------|-------|
| 1,2,3-Trichloropropane | 112.6261 | 11.15 | 0.00     | 14846 | 112.0 | 63.5   | 33.5  | 93.5  |



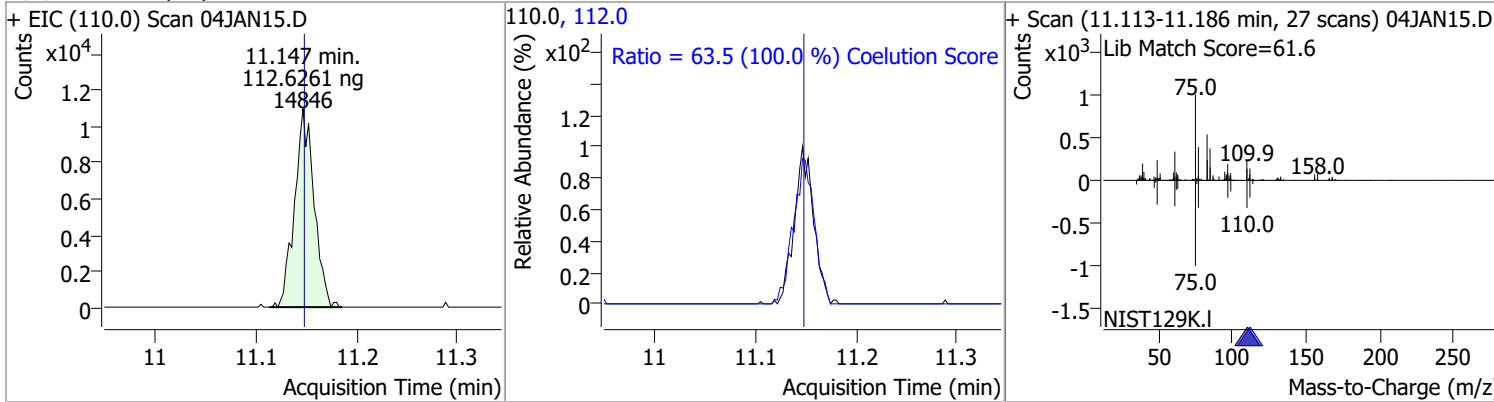


| Compound        | Conc.    | RT    | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|-----------------|----------|-------|----------|--------|------|--------|-------|-------|
| 2-Chlorotoluene | 120.2675 | 11.29 | 0.00     | 102424 | 91.0 | 282.3  | 252.3 | 312.3 |






# Quantitation Results Report (QT Reviewed)




| Compound        | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|-----------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 4-Chlorotoluene | 121.0591 | 11.40 | 0.00     | 336146 | 126.0 | 31.7   | 1.7   | 61.7  |

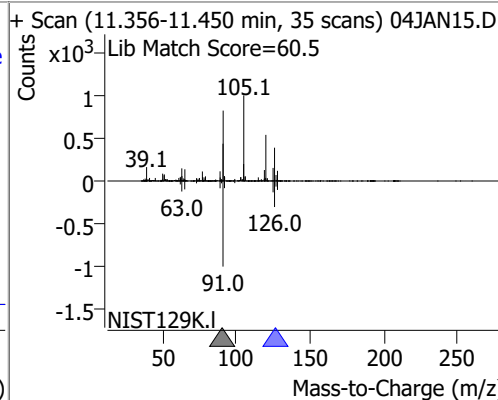

| Compound            | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,3-Dichlorobenzene | 117.4899 | 12.03 | 0.00     | 183404 | 148.0 | 63.6   | 33.6  | 93.6  |
|                     |          |       |          |        | 111.0 | 39.8   | 9.8   | 69.8  |

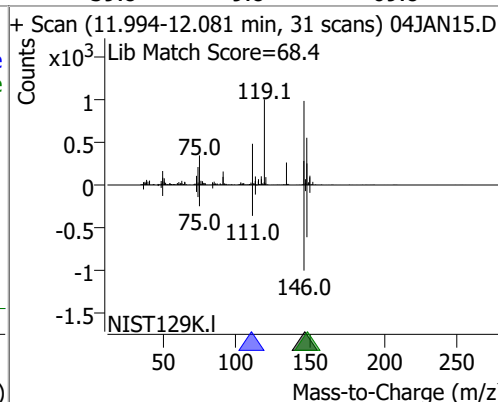




| Compound            | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,4-Dichlorobenzene | 118.7699 | 12.13 | 0.00     | 189045 | 148.0 | 63.1   | 33.1  | 93.1  |
|                     |          |       |          |        | 111.0 | 39.1   | 9.1   | 69.1  |

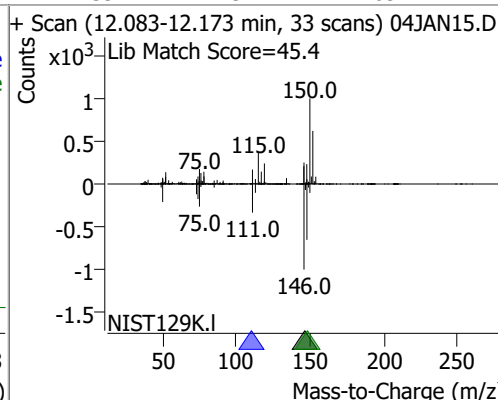


# Quantitation Results Report (QT Reviewed)

| Compound            | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,2-Dichlorobenzene | 115.4323 | 12.49 | 0.00     | 152284 | 148.0 | 63.9   | 33.9  | 93.9  |
|                     |          |       |          |        | 111.0 | 41.0   | 11.0  | 71.0  |



# Quantitation Results Report (QT Reviewed)

|                |                                     |                   |                       |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File      | 04JAN17.D                           | Operator          | MSC                   |
| Acq. Method    | 5975CACQF.M                         | Acq. Date-Time    | 1/4/2022 6:45:10 PM   |
| Sample Name    | ICAL010422_6                        | Instrument        | VOA5975C              |
| Vial           | 17                                  | Multiplier        | 1.00                  |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m  | Comment           |                       |
| Tune File      | BFB_Atune3.u                        | Tune Date         | 10/11/2021 4:02:00 PM |
| Batch Name     | VG010422_8260B.batch.bin            | Last Calib Update | 1/9/2022 8:59:52 PM   |
| Ref Library    | \\MASSHUNTER\Org\Library\NIST129K.I |                   |                       |



| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|----------|----|------|-------|-------|-------|----------|
|----------|----|------|-------|-------|-------|----------|

**Internal Standards**

|                          |        |       |        |          |    |        |
|--------------------------|--------|-------|--------|----------|----|--------|
| M Fluorobenzene          | 6.620  | 96.0  | 836278 | 250.0000 | ng | -0.003 |
| M Chlorobenzene-d5       | 9.774  | 82.0  | 316399 | 250.0000 | ng | 0.003  |
| M 1,4-Dichlorobenzene-d4 | 12.100 | 152.0 | 266553 | 250.0000 | ng | 0.000  |

**System Monitoring Compounds**

|                         |                      |       |        |                    |    |        |
|-------------------------|----------------------|-------|--------|--------------------|----|--------|
| S Dibromofluoromethane  | 5.845                | 113.0 | 204073 | 259.0223           | ng | 0.000  |
| Spiked Amount: 250.000  | Range: 80.0 - 119.0% |       |        | Recovery = 103.61% |    |        |
| S 1,2-Dichloroethane-d4 | 6.236                | 67.0  | 87876  | 258.2324           | ng | 0.003  |
| Spiked Amount: 250.000  | Range: 81.0 - 118.0% |       |        | Recovery = 103.29% |    |        |
| S Toluene-d8            | 8.319                | 98.0  | 823306 | 270.0265           | ng | 0.000  |
| Spiked Amount: 250.000  | Range: 89.0 - 112.0% |       |        | Recovery = 108.01% |    |        |
| S p-Bromofluorobenzene  | 10.951               | 95.0  | 261042 | 267.3186           | ng | -0.003 |
| Spiked Amount: 250.000  | Range: 85.0 - 114.0% |       |        | Recovery = 106.93% |    |        |

**Target Compounds**

| Compound                         | RT    | QIon  | Resp.  | Conc.     | Units | QValue |
|----------------------------------|-------|-------|--------|-----------|-------|--------|
| T Dichlorodifluoromethane        | 1.241 | 85.0  | 276334 | 252.1559  | ng    | 99     |
| T Chloromethane                  | 1.408 | 50.0  | 319523 | 240.2183  | ng    | 99     |
| T Vinyl chloride                 | 1.498 | 62.0  | 297604 | 248.6532  | ng    | 86     |
| T Bromomethane                   | 1.799 | 96.0  | 134737 | 251.7606  | ng    | 97     |
| T Chloroethane                   | 1.894 | 64.0  | 137312 | 231.7432  | ng    | 98     |
| T Trichlorofluoromethane         | 2.145 | 101.0 | 384837 | 259.0502  | ng    | 98     |
| T 1,1-Dichloroethene             | 2.702 | 96.0  | 217406 | 258.0903  | ng    | 99     |
| T Methylene chloride             | 3.333 | 49.0  | 292397 | 235.4657  | ng    | 99     |
| T trans-1,2-Dichloroethene       | 3.715 | 96.0  | 218855 | 254.6608  | ng    | 99     |
| T Methyl tert-butyl ether (MTBE) | 3.751 | 73.0  | 287653 | 258.9535  | ng    | 99     |
| T 1,1-Dichloroethane             | 4.384 | 63.0  | 413408 | 258.4325  | ng    | 99     |
| T 2,2-Dichloropropane            | 5.190 | 77.0  | 303307 | 253.0397  | ng    | 99     |
| T cis-1,2-Dichloroethene         | 5.215 | 96.0  | 228170 | 261.8706  | ng    | 96     |
| T Methyl ethyl ketone            | 5.279 | 43.0  | 317271 | 2688.2474 | ng    | 99     |
| T Bromochloromethane             | 5.519 | 128.0 | 89178  | 247.0586  | ng    | 95     |
| T Chloroform                     | 5.653 | 83.0  | 394946 | 248.0804  | ng    | 99     |

# Quantitation Results Report (QT Reviewed)

| Compound                    | RT     | QIon  | Resp.   | Conc.    | Units | Dev(Min) |
|-----------------------------|--------|-------|---------|----------|-------|----------|
| T 1,1,1-Trichloroethane     | 5.831  | 97.0  | 386005  | 258.7228 | ng    | 99       |
| T Carbon tetrachloride      | 6.026  | 117.0 | 383485  | 260.8774 | ng    | 99       |
| T 1,1-Dichloropropene       | 6.038  | 75.0  | 335741  | 264.6638 | ng    | 99       |
| T Benzene                   | 6.280  | 78.0  | 857534  | 257.5416 | ng    | 100      |
| T 1,2-Dichloroethane        | 6.322  | 62.0  | 226964  | 251.9675 | ng    | 99       |
| T Trichloroethene           | 7.030  | 95.0  | 250285  | 262.2931 | ng    | 100      |
| T 1,2-Dichloropropane       | 7.270  | 63.0  | 213800  | 254.7161 | ng    | 100      |
| T Dibromomethane            | 7.396  | 93.0  | 89483   | 252.2734 | ng    | 97       |
| T Bromodichloromethane      | 7.582  | 83.0  | 251805  | 257.2286 | ng    | 100      |
| T cis-1,3-Dichloropropene   | 8.057  | 75.0  | 293617  | 265.2863 | ng    | 99       |
| T Toluene                   | 8.386  | 92.0  | 541945  | 263.1330 | ng    | 100      |
| T trans-1,3-Dichloropropene | 8.639  | 75.0  | 207833  | 263.8027 | ng    | 98       |
| T 1,1,2-Trichloroethane     | 8.815  | 83.0  | 101888  | 248.2882 | ng    | 99       |
| T Tetrachloroethene         | 8.938  | 163.8 | 218245  | 259.7419 | ng    | 98       |
| T 1,3-Dichloropropane       | 8.980  | 76.0  | 212669  | 263.4754 | ng    | 98       |
| T Chlorodibromomethane      | 9.203  | 129.0 | 165695  | 258.3535 | ng    | 100      |
| T 1,2-Dibromoethane         | 9.306  | 107.0 | 115714  | 257.8887 | ng    | 100      |
| T Chlorobenzene             | 9.802  | 112.0 | 582326  | 258.2544 | ng    | 100      |
| T 1,1,1,2-Tetrachloroethane | 9.891  | 131.0 | 200859  | 254.8274 | ng    | 100      |
| T Ethylbenzene              | 9.919  | 91.0  | 1043443 | 266.8193 | ng    | 100      |
| T m+p-Xylenes               | 10.039 | 106.0 | 825866  | 543.4262 | ng    | 100      |
| T o-Xylene                  | 10.430 | 106.0 | 365914  | 270.4636 | ng    | 100      |
| T Styrene                   | 10.446 | 104.0 | 605646  | 278.0455 | ng    | 99       |
| T Bromoform                 | 10.628 | 172.5 | 87836   | 257.5099 | ng    | 100      |
| T Bromobenzene              | 11.093 | 156.0 | 227127  | 263.2944 | ng    | 99       |
| T 1,1,2,2-Tetrachloroethane | 11.113 | 83.0  | 124205  | 250.1577 | ng    | 97       |
| T 1,2,3-Trichloropropane    | 11.152 | 110.0 | 33115   | 249.2635 | ng    | 97       |
| T 2-Chlorotoluene           | 11.291 | 126.0 | 229396  | 267.2616 | ng    | 99       |
| T 4-Chlorotoluene           | 11.400 | 91.0  | 748435  | 267.4409 | ng    | 99       |
| T 1,3-Dichlorobenzene       | 12.033 | 146.0 | 406895  | 258.6297 | ng    | 99       |
| T 1,4-Dichlorobenzene       | 12.122 | 146.0 | 408934  | 254.9170 | ng    | 98       |
| T 1,2-Dichlorobenzene       | 12.493 | 146.0 | 342576  | 257.6524 | ng    | 99       |

(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (\*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak


# Quantitation Results Report (QT Reviewed)

| Compound                    | Conc.    | RT   | Dev(Min)   | Resp.  | QIon | QRatio                                       | Lower | Upper |
|-----------------------------|----------|------|------------|--------|------|----------------------------------------------|-------|-------|
| Dichlorodifluoromethane     | 252.1559 | 1.24 | 0.00       | 276334 | 87.0 | 31.6                                         | 2.3   | 62.3  |
| + EIC (85.0) Scan 04JAN17.D |          |      | 85.0, 87.0 |        |      | + Scan (1.216-1.344 min, 47 scans) 04JAN17.D |       |       |
|                             |          |      |            |        |      |                                              |       |       |
| Chloromethane               | 240.2183 | 1.41 | 0.00       | 319523 | 52.0 | 32.9                                         | 2.1   | 62.1  |
| + EIC (50.0) Scan 04JAN17.D |          |      | 50.0, 52.0 |        |      | + Scan (1.367-1.537 min, 62 scans) 04JAN17.D |       |       |
|                             |          |      |            |        |      |                                              |       |       |
| Vinyl chloride              | 248.6532 | 1.50 | 0.00       | 297604 | 64.0 | 37.7                                         | 0.0   | 59.9  |
| + EIC (62.0) Scan 04JAN17.D |          |      | 62.0, 64.0 |        |      | + Scan (1.467-1.615 min, 54 scans) 04JAN17.D |       |       |
|                             |          |      |            |        |      |                                              |       |       |
| Bromomethane                | 251.7606 | 1.80 | 0.00       | 134737 | 94.0 | 107.5                                        | 74.6  | 134.6 |
| + EIC (96.0) Scan 04JAN17.D |          |      | 96.0, 94.0 |        |      | + Scan (1.760-1.919 min, 58 scans) 04JAN17.D |       |       |
|                             |          |      |            |        |      |                                              |       |       |




# Quantitation Results Report (QT Reviewed)


| Compound     | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------|----------|------|----------|--------|------|--------|-------|-------|
| Chloroethane | 231.7432 | 1.89 | 0.00     | 137312 | 66.0 | 31.0   | 0.1   | 60.1  |

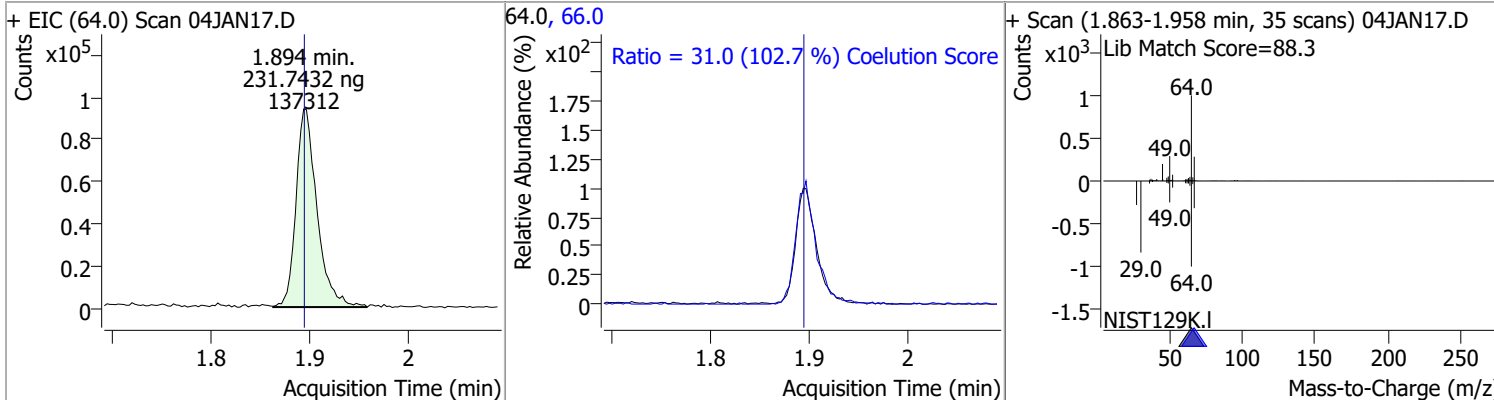


|                        |          |      |      |        |       |      |      |      |
|------------------------|----------|------|------|--------|-------|------|------|------|
| Trichlorofluoromethane | 259.0502 | 2.14 | 0.00 | 384837 | 103.0 | 65.6 | 34.2 | 94.2 |
|------------------------|----------|------|------|--------|-------|------|------|------|

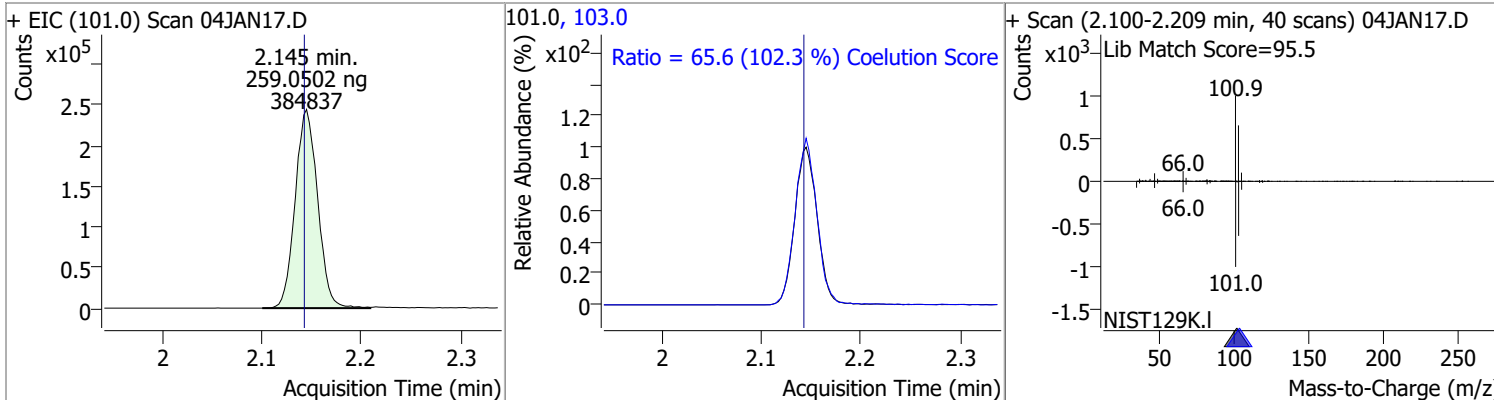

|                    |          |      |      |        |      |       |       |       |
|--------------------|----------|------|------|--------|------|-------|-------|-------|
| 1,1-Dichloroethene | 258.0903 | 2.70 | 0.01 | 217406 | 61.0 | 181.2 | 150.3 | 210.3 |
|                    |          |      |      |        | 63.0 | 56.8  | 26.7  | 86.7  |

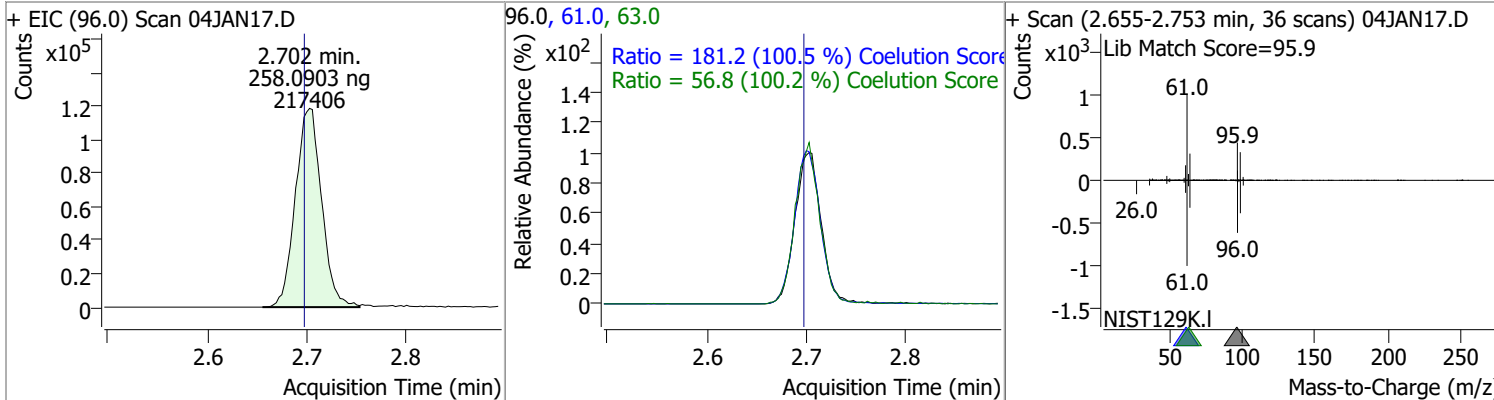


|                    |          |      |      |        |      |      |      |      |
|--------------------|----------|------|------|--------|------|------|------|------|
| Methylene chloride | 235.4657 | 3.33 | 0.00 | 292397 | 84.0 | 66.4 | 36.9 | 96.9 |
|                    |          |      |      |        | 86.0 | 42.7 | 14.3 | 74.3 |

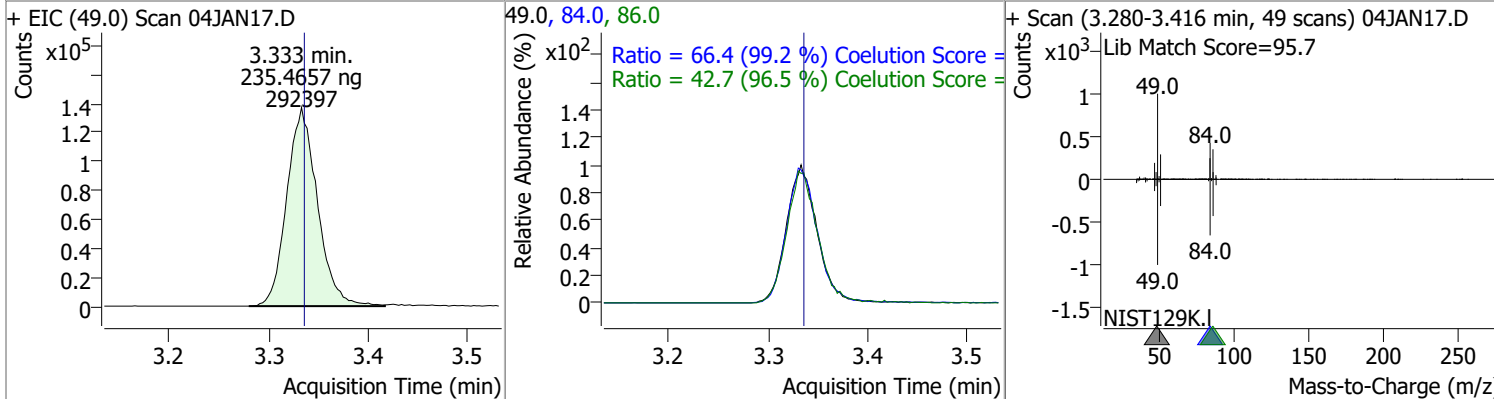


# Quantitation Results Report (QT Reviewed)


| Compound                 | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------------|----------|------|----------|--------|------|--------|-------|-------|
| trans-1,2-Dichloroethene | 254.6608 | 3.71 | 0.00     | 218855 | 61.0 | 153.9  | 123.9 | 183.9 |
|                          |          |      |          |        | 98.0 | 63.7   | 35.7  | 95.7  |

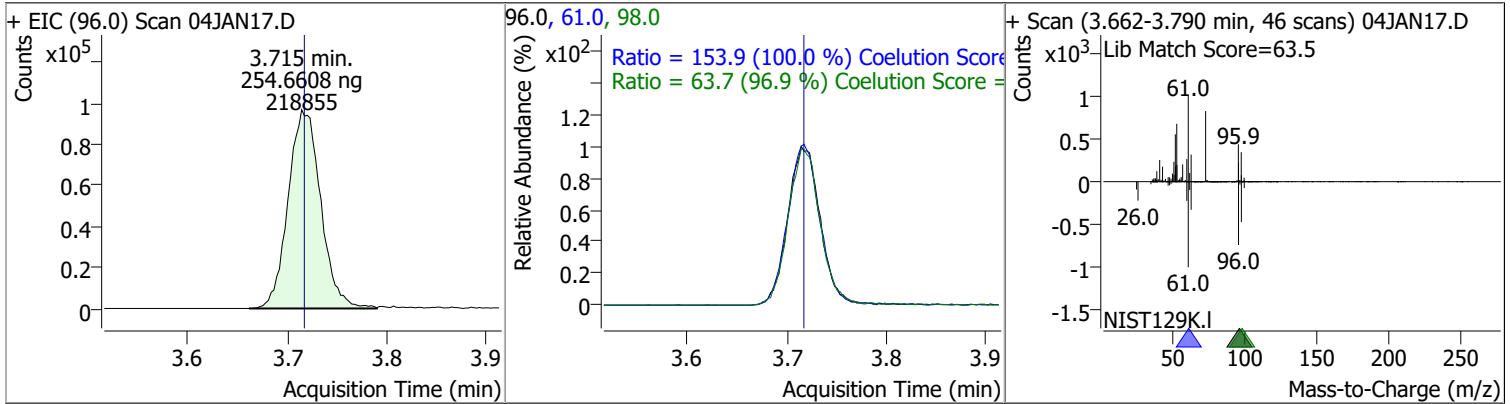

| Compound                       | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------------------|----------|------|----------|--------|------|--------|-------|-------|
| Methyl tert-butyl ether (MTBE) | 258.9535 | 3.75 | 0.00     | 287653 | 57.0 | 25.3   | 0.0   | 54.6  |

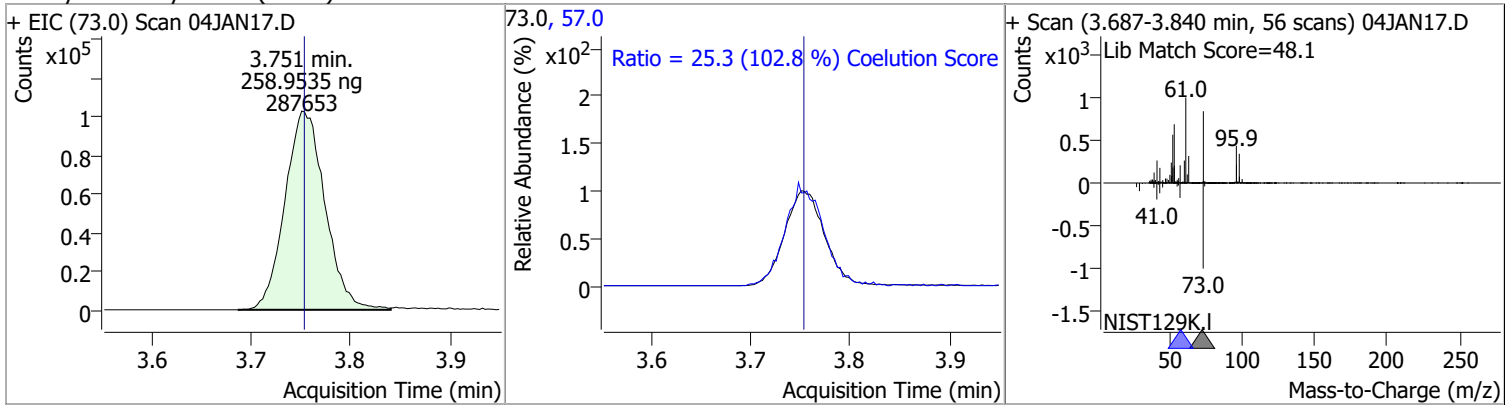


| Compound           | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1-Dichloroethane | 258.4325 | 4.38 | 0.01     | 413408 | 65.0 | 31.4   | 2.1   | 62.1  |
|                    |          |      |          |        | 83.0 | 13.2   | 0.0   | 43.7  |




# Quantitation Results Report (QT Reviewed)


| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 2,2-Dichloropropane | 253.0397 | 5.19 | -0.01    | 303307 | 41.0 | 67.7   | 36.5  | 96.5  |
|                     |          |      |          |        | 97.0 | 22.8   | 0.0   | 53.2  |

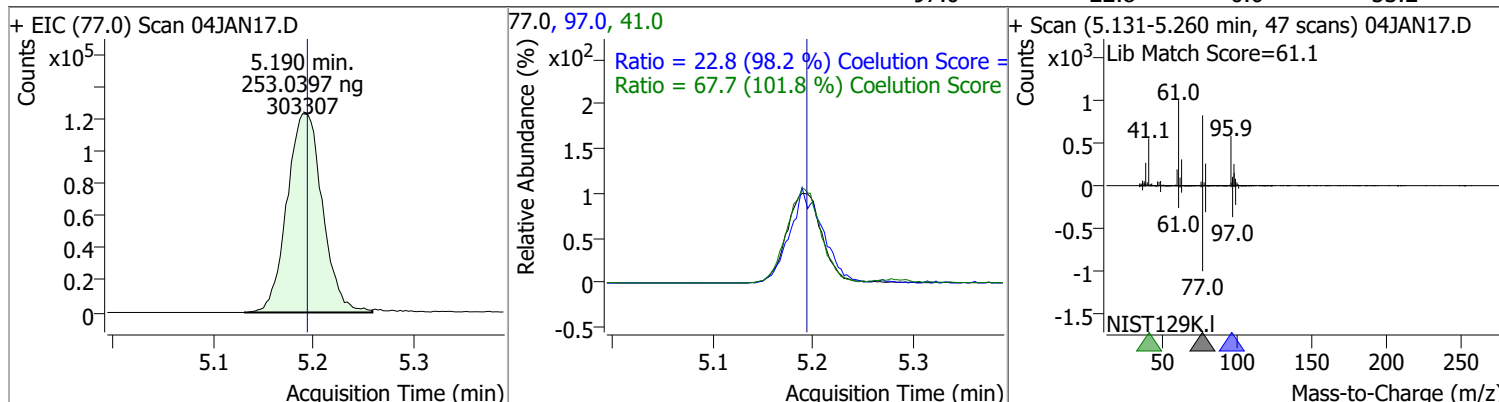


| Compound               | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,2-Dichloroethene | 261.8706 | 5.21 | 0.00     | 228170 | 61.0 | 161.6  | 137.2 | 197.2 |
|                        |          |      |          |        | 98.0 | 65.6   | 37.3  | 97.3  |

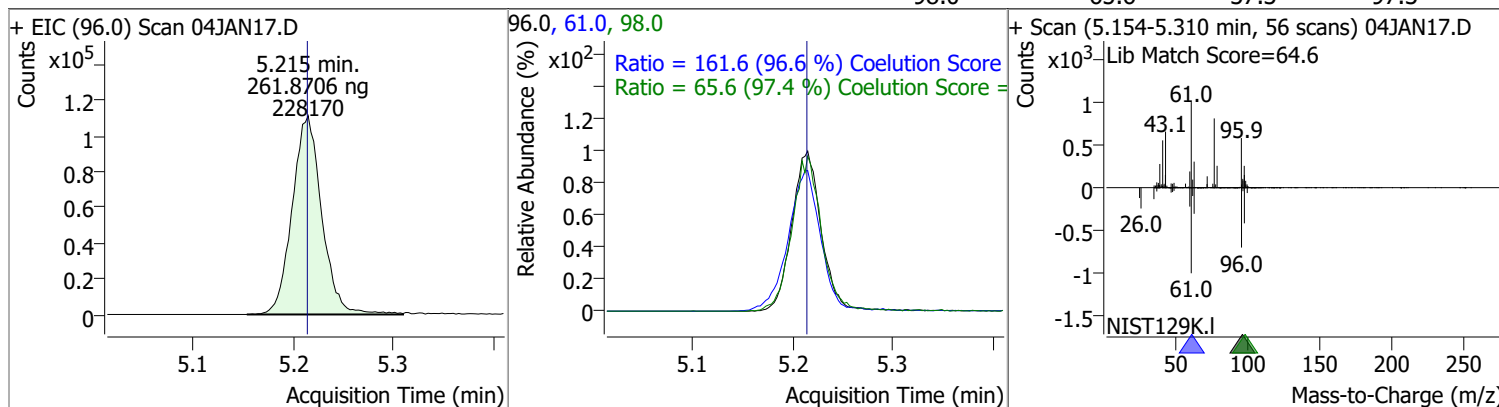

| Compound            | Conc.     | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|-----------|------|----------|--------|------|--------|-------|-------|
| Methyl ethyl ketone | 2688.2474 | 5.28 | 0.00     | 317271 | 72.0 | 20.8   | 0.0   | 51.3  |

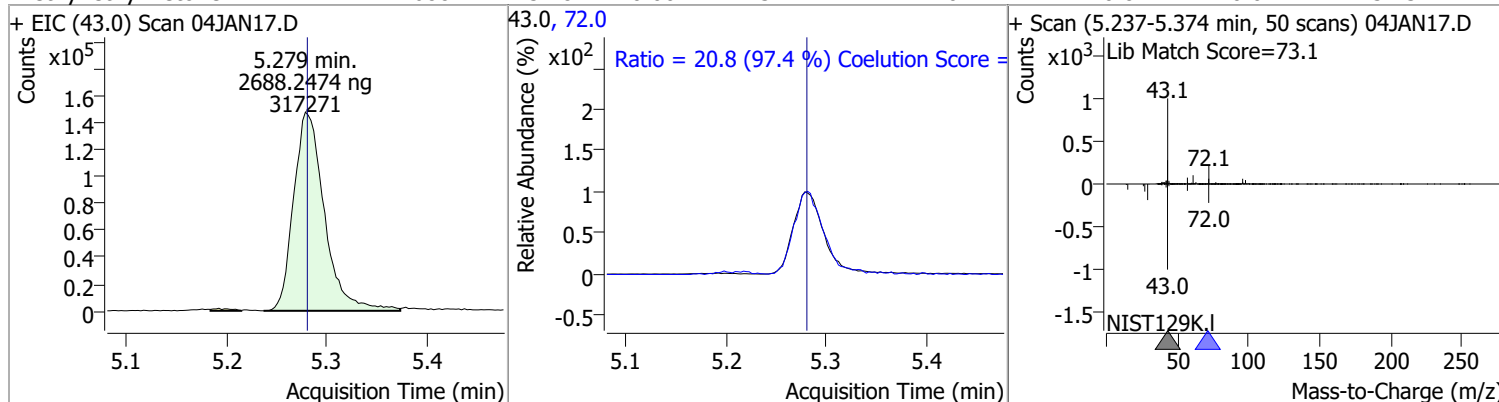


| Compound           | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|-------|------|--------|-------|-------|
| Bromochloromethane | 247.0586 | 5.52 | 0.00     | 89178 | 49.0 | 190.0  | 152.9 | 212.9 |

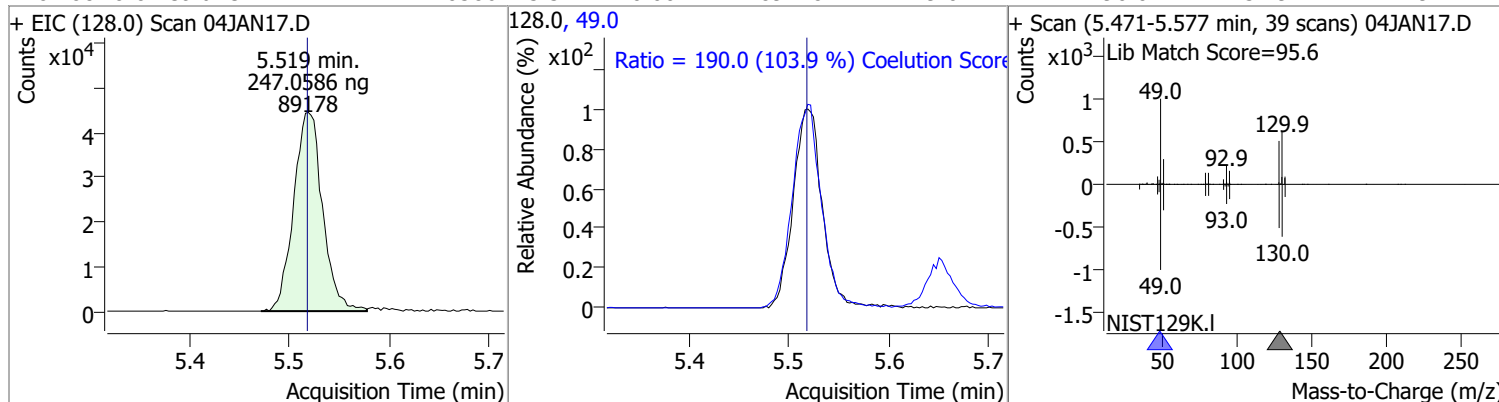


# Quantitation Results Report (QT Reviewed)


| Compound   | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|------|--------|-------|-------|
| Chloroform | 248.0804 | 5.65 | 0.00     | 394946 | 85.0 | 64.9   | 36.0  | 96.0  |




| Compound              | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1,1-Trichloroethane | 258.7228 | 5.83 | 0.00     | 386005 | 99.0 | 64.4   | 34.7  | 94.7  |
|                       |          |      |          |        | 61.0 | 48.7   | 18.1  | 78.1  |



| Compound             | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Dibromofluoromethane | 259.0223 | 5.85 | 0.00     | 204073 | 191.5 | 22.5   | 0.0   | 53.1  |




| Compound             | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Carbon tetrachloride | 260.8774 | 6.03 | 0.00     | 383485 | 119.0 | 97.0   | 67.2  | 127.2 |
|                      |          |      |          |        | 121.0 | 30.9   | 0.1   | 60.1  |




# Quantitation Results Report (QT Reviewed)


| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|-------|--------|-------|-------|
| 1,1-Dichloropropene | 264.6638 | 6.04 | 0.00     | 335741 | 110.0 | 35.6   | 5.9   | 65.9  |
|                     |          |      |          |        | 77.0  | 30.7   | 0.1   | 60.1  |

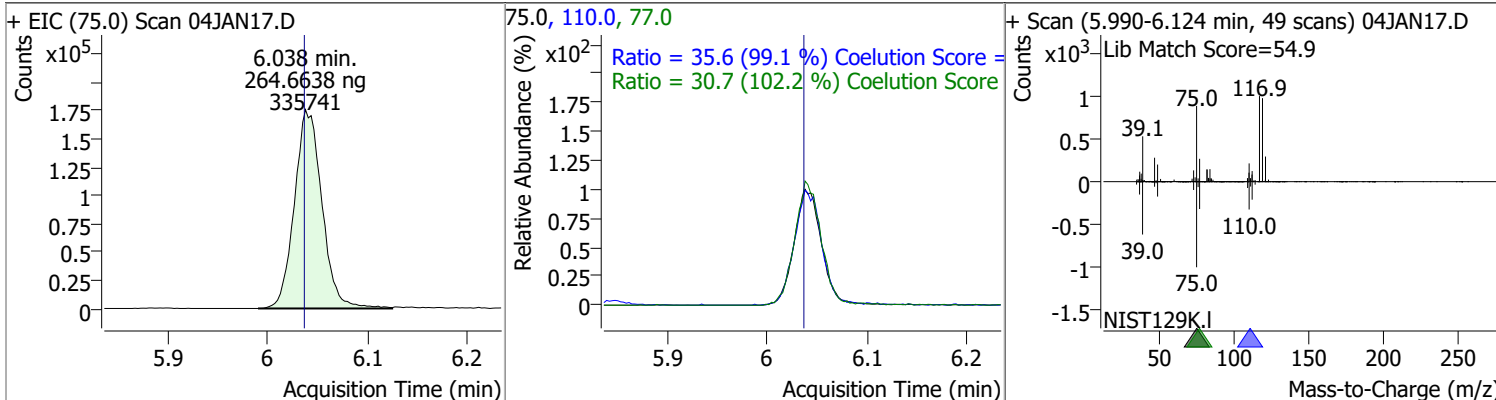


| Compound              | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 258.2324 | 6.24 | 0.00     | 87876 | 65.0 | 193.6  | 166.5 | 226.5 |

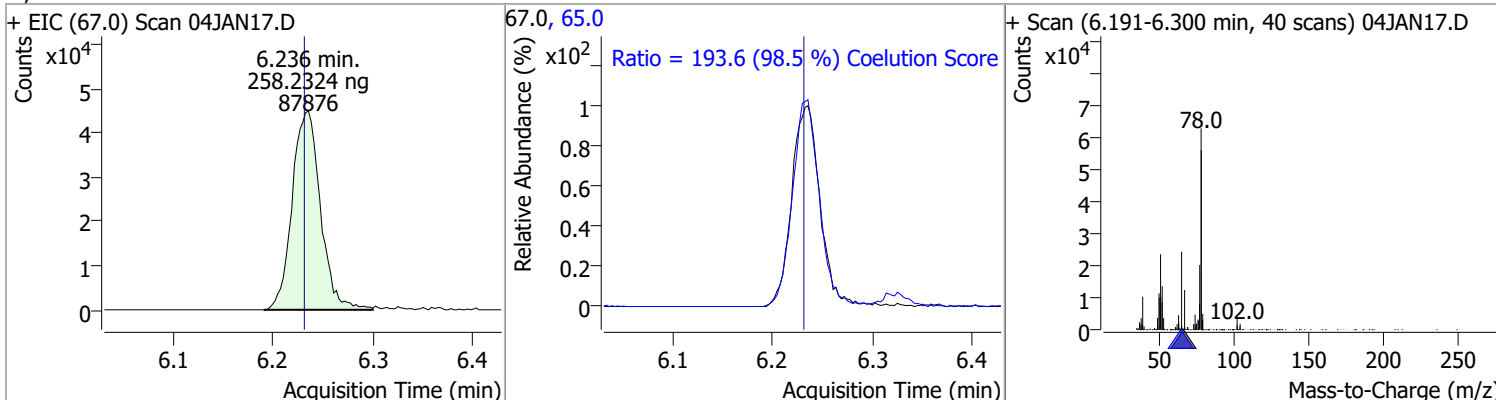

| Compound | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|----------|----------|------|----------|--------|------|--------|-------|-------|
| Benzene  | 257.5416 | 6.28 | 0.00     | 857534 | 77.0 | 23.6   | 0.0   | 53.5  |

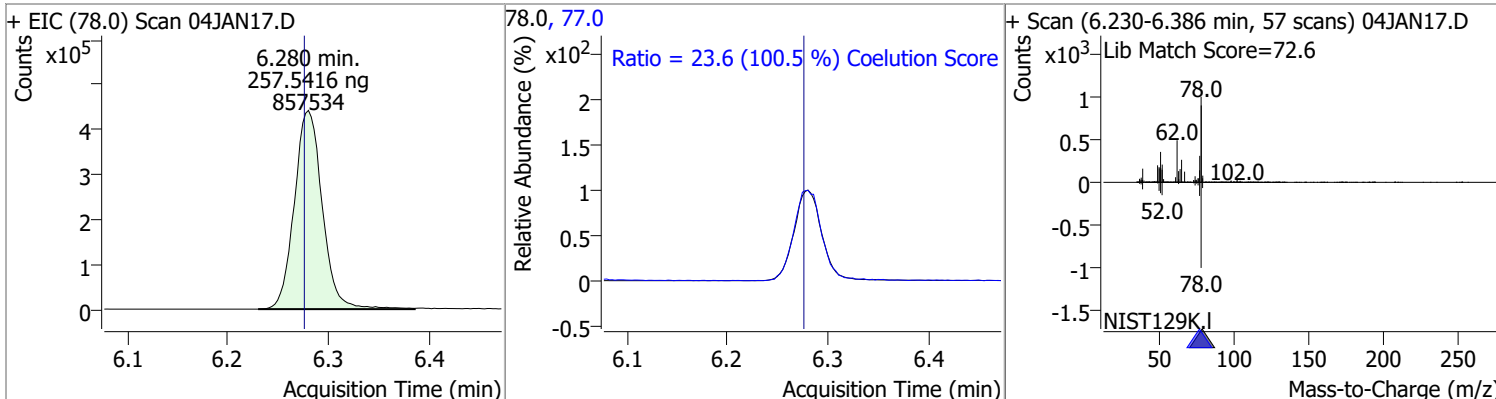


| Compound           | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloroethane | 251.9675 | 6.32 | 0.00     | 226964 | 64.0 | 30.6   | 0.0   | 59.9  |
|                    |          |      |          |        | 98.0 | 7.4    | 0.0   | 37.6  |

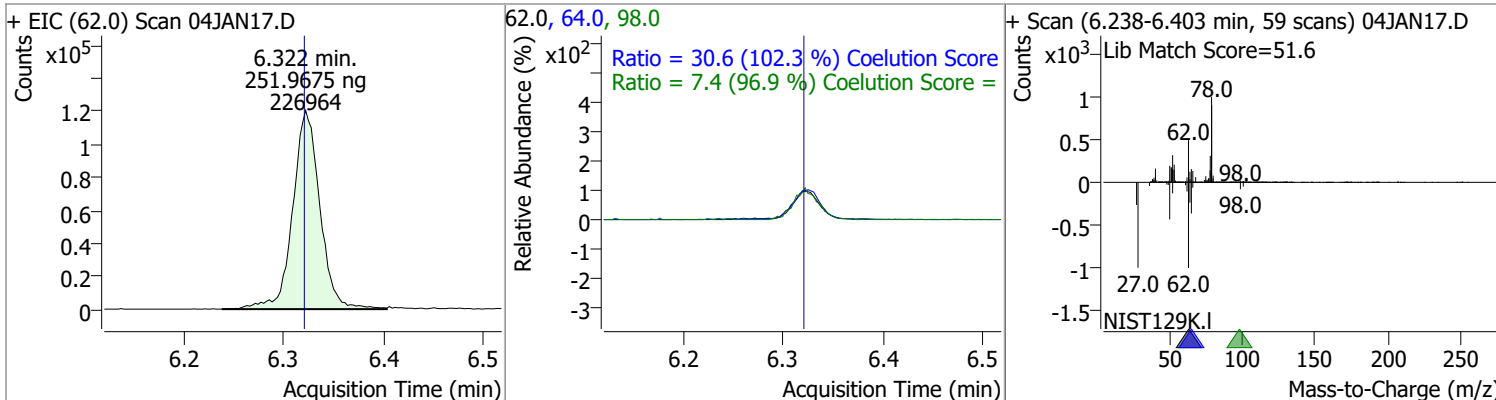


# Quantitation Results Report (QT Reviewed)


| Compound        | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|-----------------|----------|------|----------|--------|-------|--------|-------|-------|
| Trichloroethene | 262.2931 | 7.03 | 0.00     | 250285 | 130.0 | 101.7  | 71.5  | 131.5 |
|                 |          |      |          |        | 97.0  | 64.5   | 34.1  | 94.1  |

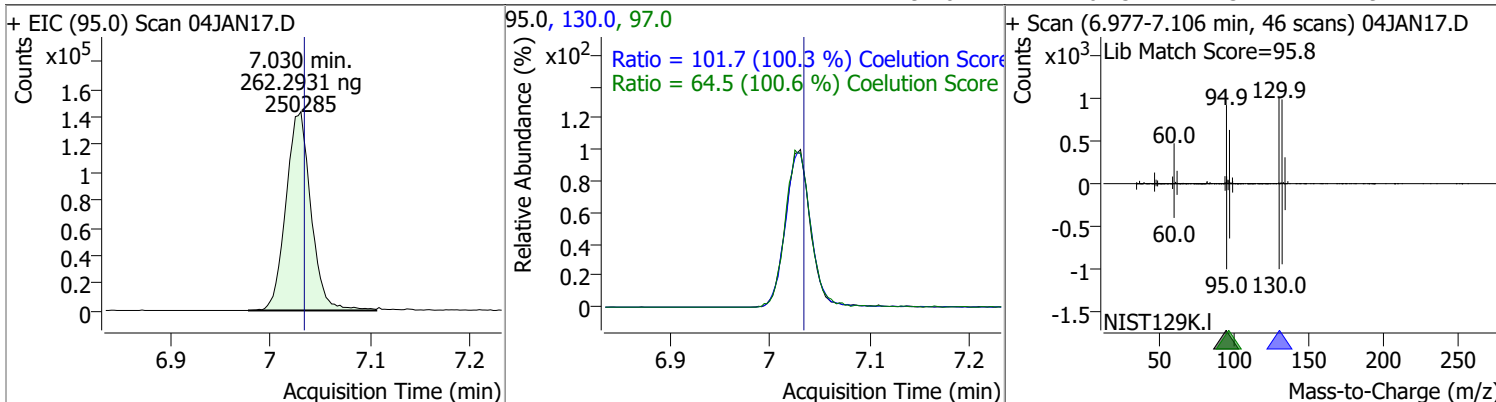

| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloropropane | 254.7161 | 7.27 | 0.00     | 213800 | 76.0 | 38.5   | 8.2   | 68.2  |




| Compound       | Conc.    | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|----------------|----------|------|----------|-------|-------|--------|-------|-------|
| Dibromomethane | 252.2734 | 7.40 | 0.00     | 89483 | 173.5 | 108.9  | 83.7  | 143.7 |
|                |          |      |          |       | 95.0  | 83.1   | 52.2  | 112.2 |

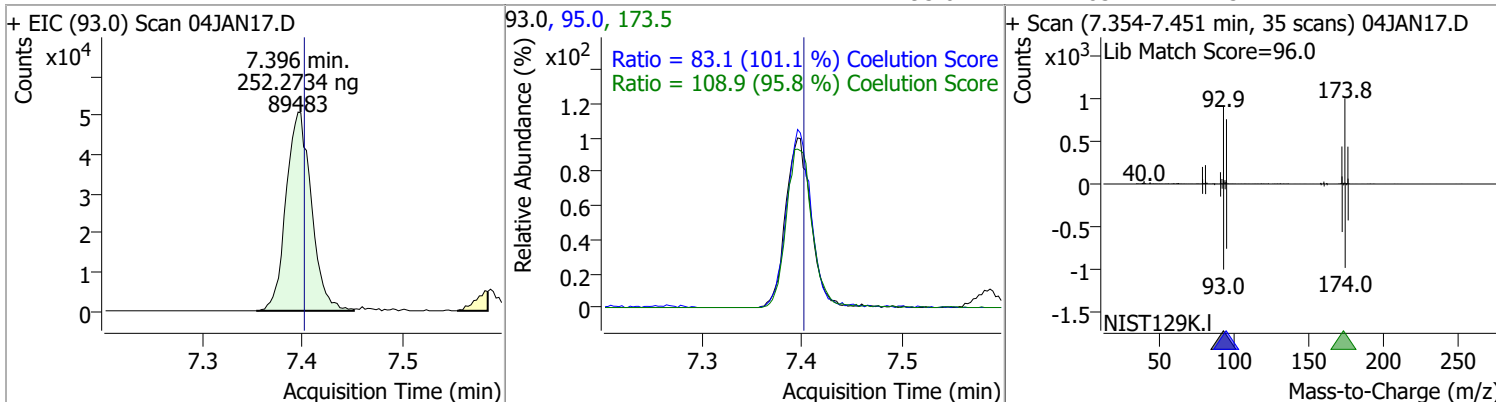


# Quantitation Results Report (QT Reviewed)


| Compound             | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Bromodichloromethane | 257.2286 | 7.58 | 0.00     | 251805 | 85.0  | 64.3   | 34.5  | 94.5  |
|                      |          |      |          |        | 127.0 | 9.3    | 0.0   | 39.6  |

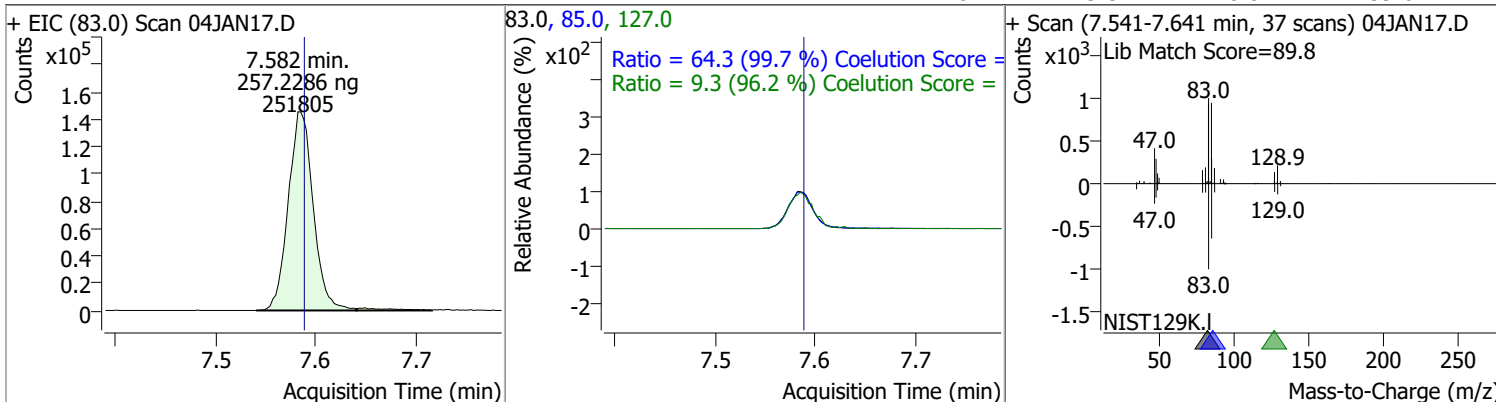

| Compound                | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|-------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,3-Dichloropropene | 265.2863 | 8.06 | 0.00     | 293617 | 39.0 | 53.0   | 23.3  | 83.3  |
|                         |          |      |          |        | 77.0 | 31.6   | 1.0   | 61.0  |

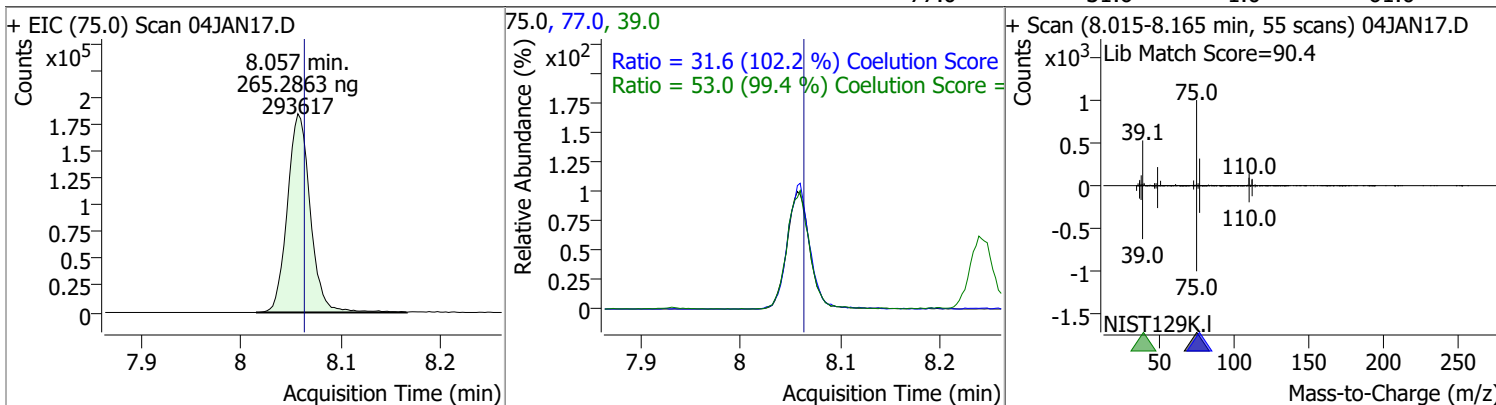

| Compound   | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 270.0265 | 8.32 | 0.00     | 823306 | 100.0 | 63.9   | 34.4  | 94.4  |
|            |          |      |          |        | 99.0  | 9.4    | 0.0   | 39.6  |

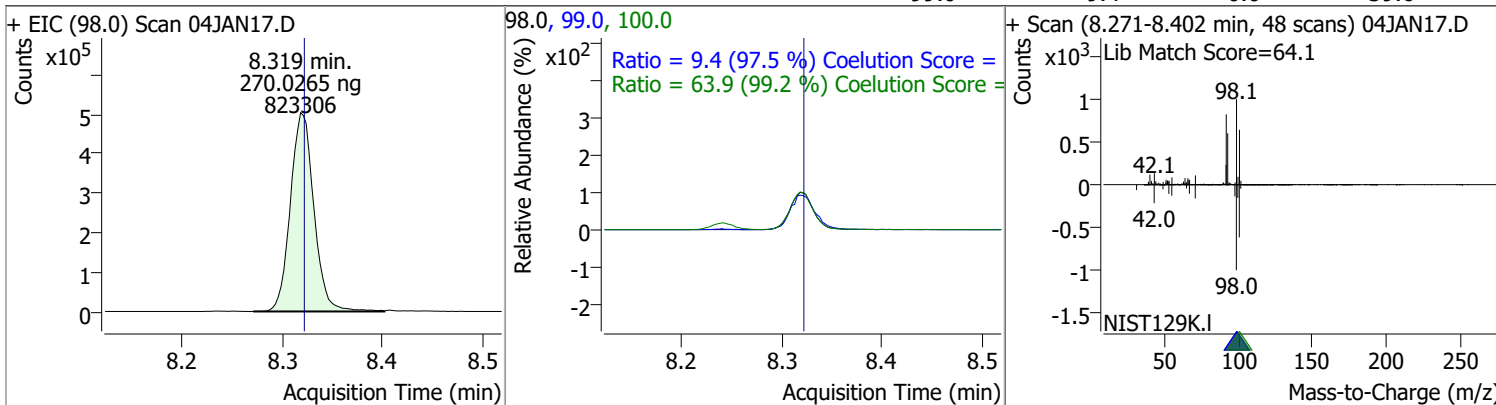


# Quantitation Results Report (QT Reviewed)

| Compound                    | Conc.    | RT   | Dev(Min)                               | Resp.  | QIon | QRatio                                       | Lower | Upper |
|-----------------------------|----------|------|----------------------------------------|--------|------|----------------------------------------------|-------|-------|
| Toluene                     | 263.1330 | 8.39 | 0.00                                   | 541945 | 91.0 | 175.7                                        | 145.8 | 205.8 |
| + EIC (92.0) Scan 04JAN17.D |          |      | 92.0, 91.0                             |        |      | + Scan (8.344-8.453 min, 40 scans) 04JAN17.D |       |       |
|                             |          |      |                                        |        |      |                                              |       |       |
|                             |          |      | Ratio = 175.7 (99.9 %) Coelution Score |        |      |                                              |       |       |
| trans-1,3-Dichloropropene   | 263.8027 | 8.64 | 0.00                                   | 207833 | 39.0 | 53.9                                         | 23.4  | 83.4  |
| + EIC (75.0) Scan 04JAN17.D |          |      | 75.0, 77.0, 39.0                       |        |      | + Scan (8.598-8.687 min, 32 scans) 04JAN17.D |       |       |
|                             |          |      |                                        |        |      |                                              |       |       |
|                             |          |      | Ratio = 35.1 (108.3 %) Coelution Score |        |      |                                              |       |       |
|                             |          |      | Ratio = 53.9 (101.1 %) Coelution Score |        |      |                                              |       |       |
| 1,1,2-Trichloroethane       | 248.2882 | 8.82 | 0.00                                   | 101888 | 97.0 | 114.4                                        | 84.6  | 144.6 |
| + EIC (83.0) Scan 04JAN17.D |          |      | 83.0, 97.0, 85.0                       |        |      | + Scan (8.776-8.879 min, 38 scans) 04JAN17.D |       |       |
|                             |          |      |                                        |        |      |                                              |       |       |
|                             |          |      | Ratio = 114.4 (99.8 %) Coelution Score |        |      |                                              |       |       |
|                             |          |      | Ratio = 65.7 (97.1 %) Coelution Score  |        |      |                                              |       |       |




# Quantitation Results Report (QT Reviewed)


| Compound          | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|-------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Tetrachloroethene | 259.7419 | 8.94 | 0.00     | 218245 | 165.8 | 126.5  | 98.6  | 158.6 |
|                   |          |      |          |        | 129.0 | 90.3   | 61.5  | 121.5 |




| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,3-Dichloropropane | 263.4754 | 8.98 | 0.00     | 212669 | 78.0 | 31.9   | 2.9   | 62.9  |







| Compound             | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Chlorodibromomethane | 258.3535 | 9.20 | 0.00     | 165695 | 127.0 | 77.8   | 48.0  | 108.0 |



| Compound          | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|-------------------|----------|------|----------|--------|-------|--------|-------|-------|
| 1,2-Dibromoethane | 257.8887 | 9.31 | 0.00     | 115714 | 109.0 | 94.6   | 64.5  | 124.5 |




# Quantitation Results Report (QT Reviewed)




# Quantitation Results Report (QT Reviewed)


| Compound | Conc.    | RT    | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|----------|----------|-------|----------|--------|------|--------|-------|-------|
| o-Xylene | 270.4636 | 10.43 | 0.00     | 365914 | 91.0 | 213.0  | 183.1 | 243.1 |




| Compound | Conc.    | RT    | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|----------|----------|-------|----------|--------|------|--------|-------|-------|
| Styrene  | 278.0455 | 10.45 | 0.00     | 605646 | 78.0 | 50.3   | 19.6  | 79.6  |



| Compound  | Conc.    | RT    | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|-----------|----------|-------|----------|-------|-------|--------|-------|-------|
| Bromoform | 257.5099 | 10.63 | 0.00     | 87836 | 170.5 | 51.9   | 22.1  | 82.1  |
|           |          |       |          |       | 174.5 | 50.3   | 20.1  | 80.1  |




| Compound             | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 267.3186 | 10.95 | 0.00     | 261042 | 174.0 | 93.1   | 61.7  | 121.7 |
|                      |          |       |          |        | 176.0 | 89.6   | 60.6  | 120.6 |




# Quantitation Results Report (QT Reviewed)


| Compound     | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|--------------|----------|-------|----------|--------|-------|--------|-------|-------|
| Bromobenzene | 263.2944 | 11.09 | 0.00     | 227127 | 77.0  | 143.1  | 115.7 | 175.7 |
|              |          |       |          |        | 158.0 | 96.5   | 66.5  | 126.5 |

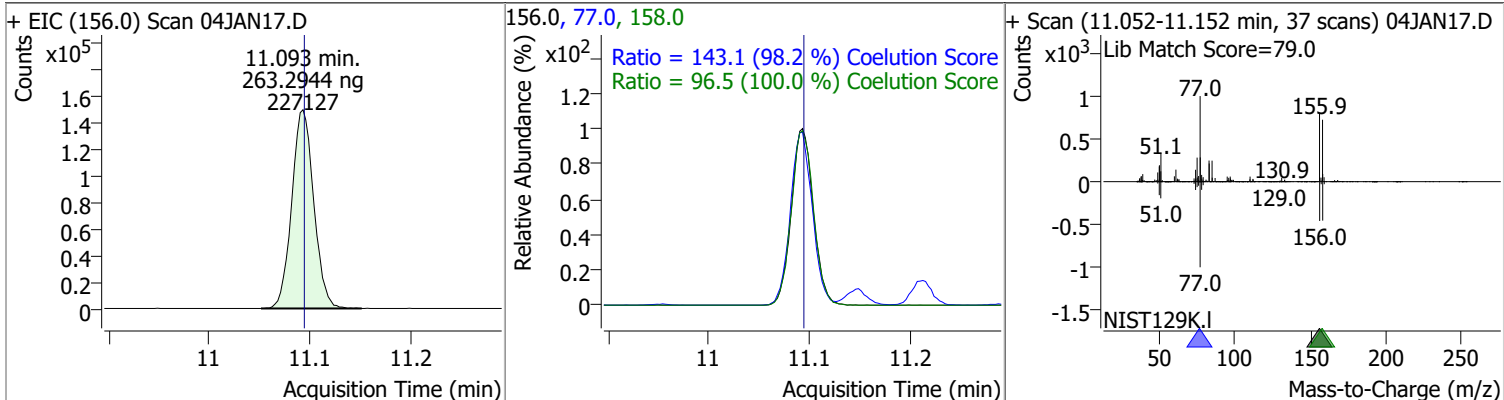


| Compound                  | Conc.    | RT    | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------------|----------|-------|----------|--------|------|--------|-------|-------|
| 1,1,2,2-Tetrachloroethane | 250.1577 | 11.11 | 0.00     | 124205 | 85.0 | 64.1   | 36.2  | 96.2  |

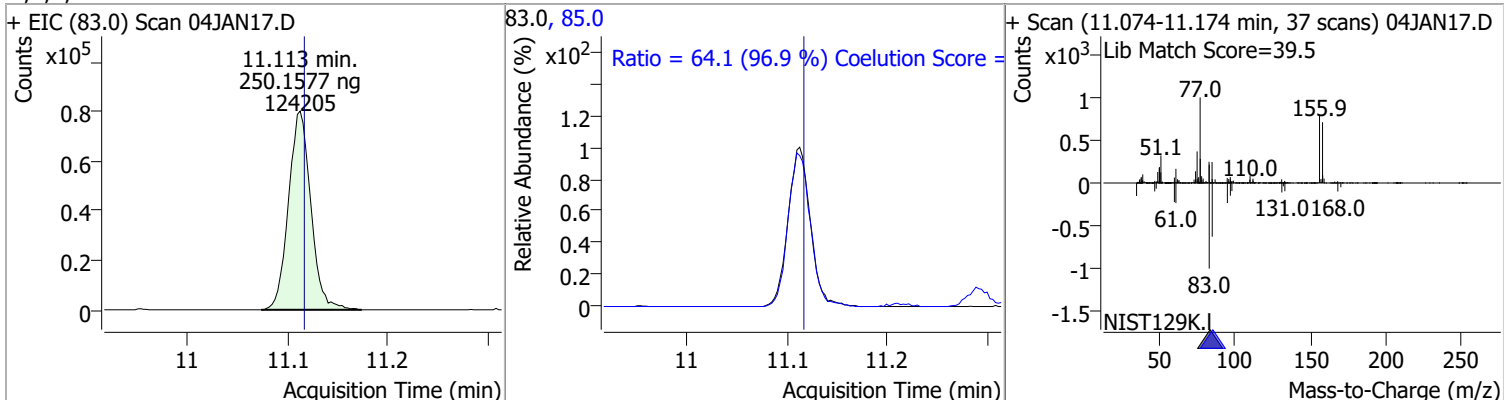

| Compound               | Conc.    | RT    | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|------------------------|----------|-------|----------|-------|-------|--------|-------|-------|
| 1,2,3-Trichloropropane | 249.2635 | 11.15 | 0.01     | 33115 | 112.0 | 65.5   | 33.5  | 93.5  |



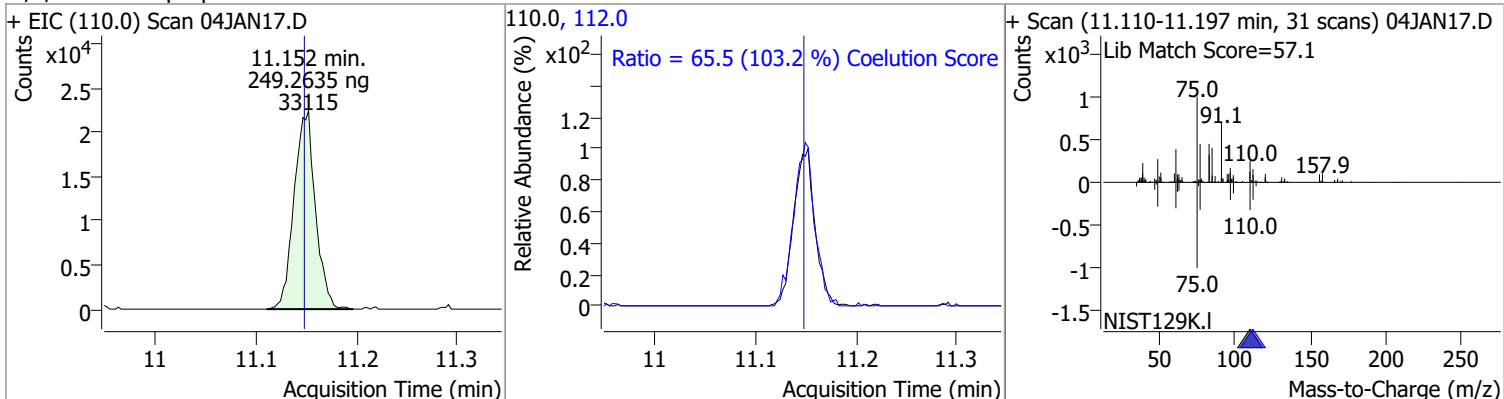


| Compound        | Conc.    | RT    | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|-----------------|----------|-------|----------|--------|------|--------|-------|-------|
| 2-Chlorotoluene | 267.2616 | 11.29 | 0.00     | 229396 | 91.0 | 283.3  | 252.3 | 312.3 |



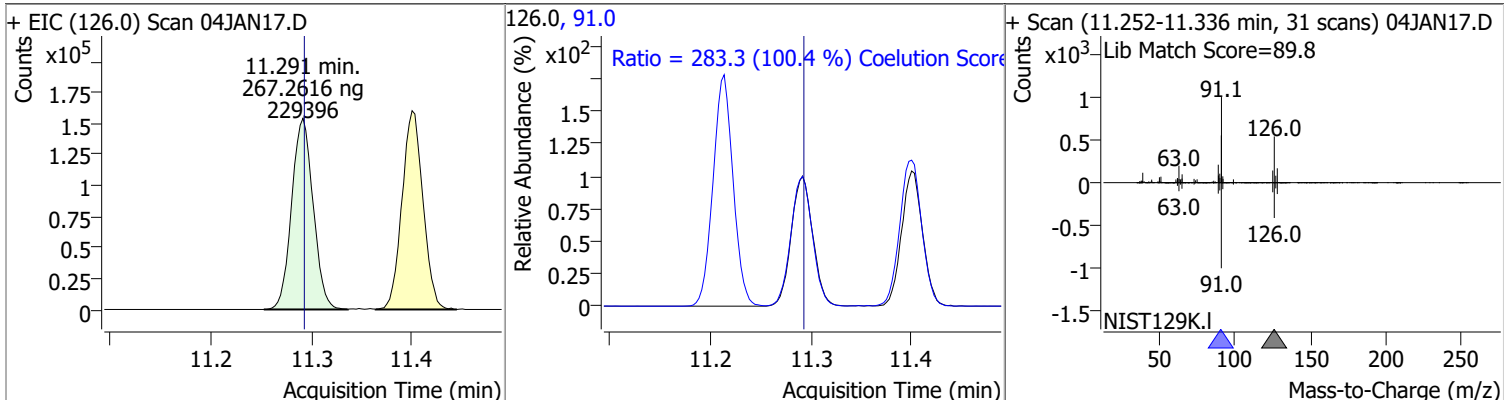


# Quantitation Results Report (QT Reviewed)




| Compound        | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|-----------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 4-Chlorotoluene | 267.4409 | 11.40 | 0.00     | 748435 | 126.0 | 31.1   | 1.7   | 61.7  |



| Compound            | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,3-Dichlorobenzene | 258.6297 | 12.03 | 0.00     | 406895 | 148.0 | 63.3   | 33.6  | 93.6  |
|                     |          |       |          |        | 111.0 | 39.0   | 9.8   | 69.8  |






| Compound            | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,4-Dichlorobenzene | 254.9170 | 12.12 | 0.00     | 408934 | 148.0 | 64.9   | 33.1  | 93.1  |
|                     |          |       |          |        | 111.0 | 38.3   | 9.1   | 69.1  |




# Quantitation Results Report (QT Reviewed)

| Compound            | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,2-Dichlorobenzene | 257.6524 | 12.49 | 0.00     | 342576 | 148.0 | 63.4   | 33.9  | 93.9  |
|                     |          |       |          |        | 111.0 | 40.5   | 11.0  | 71.0  |

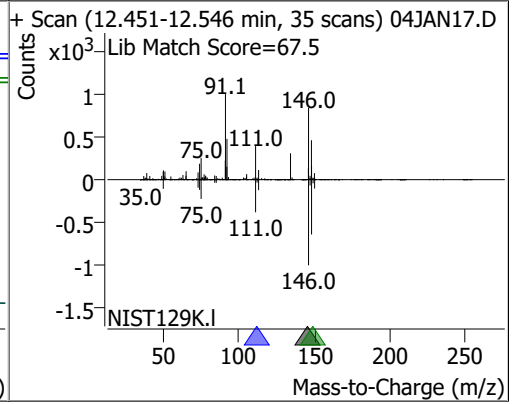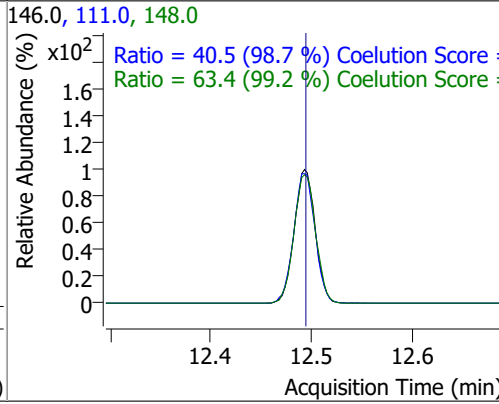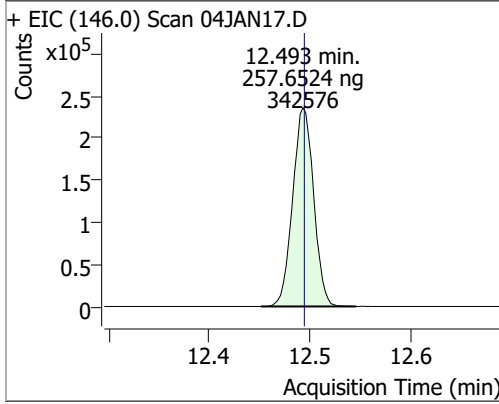

# Quantitation Results Report (QT Reviewed)

Data File 04JAN19.D Operator MSC  
Acq. Method 5975CACQF.M Acq. Date-Time 1/4/2022 7:39:45 PM  
Sample Name ICAL010422\_7 Instrument VOA5975C  
Vial 19 Multiplier 1.00  
DA Method File VOA5975C\_8260B\_SHT\_DoD\_L4\_010422.m Comment  
Tune File BFB\_Atune3.u Tune Date 10/11/2021 4:02:00 PM  
Batch Name VG010422\_8260B.batch.bin Last Calib Update 1/9/2022 8:59:52 PM  
Ref Library \\MASSHUNTER\Org\Library\NIST129K.I



| Compound                           | RT                   | QIon  | Resp.   | Conc.              | Units | Dev(Min) |
|------------------------------------|----------------------|-------|---------|--------------------|-------|----------|
| <b>Internal Standards</b>          |                      |       |         |                    |       |          |
| M Fluorobenzene                    | 6.621                | 96.0  | 841876  | 250.0000           | ng    | -0.003   |
| M Chlorobenzene-d5                 | 9.772                | 82.0  | 314668  | 250.0000           | ng    | 0.000    |
| M 1,4-Dichlorobenzene-d4           | 12.100               | 152.0 | 266611  | 250.0000           | ng    | 0.000    |
| <b>System Monitoring Compounds</b> |                      |       |         |                    |       |          |
| S Dibromofluoromethane             | 5.848                | 113.0 | 305158  | 384.7503           | ng    | 0.003    |
| Spiked Amount: 250.000             | Range: 80.0 - 119.0% |       |         | Recovery = 153.90% | *     |          |
| S 1,2-Dichloroethane-d4            | 6.233                | 67.0  | 129608  | 378.3335           | ng    | 0.000    |
| Spiked Amount: 250.000             | Range: 81.0 - 118.0% |       |         | Recovery = 151.33% | *     |          |
| S Toluene-d8                       | 8.322                | 98.0  | 1229775 | 405.5583           | ng    | 0.003    |
| Spiked Amount: 250.000             | Range: 89.0 - 112.0% |       |         | Recovery = 162.22% | *     |          |
| S p-Bromofluorobenzene             | 10.951               | 95.0  | 385474  | 394.6566           | ng    | -0.003   |
| Spiked Amount: 250.000             | Range: 85.0 - 114.0% |       |         | Recovery = 157.86% | *     |          |
| <b>Target Compounds</b>            |                      |       |         |                    |       |          |
| T Dichlorodifluoromethane          | 1.241                | 85.0  | 412544  | 373.9449           | ng    | 100      |
| T Chloromethane                    | 1.409                | 50.0  | 471454  | 352.0836           | ng    | 99       |
| T Vinyl chloride                   | 1.498                | 62.0  | 448643  | 372.3564           | ng    | 95       |
| T Bromomethane                     | 1.796                | 96.0  | 207491  | 385.1259           | ng    | 98       |
| T Chloroethane                     | 1.897                | 64.0  | 217393  | 364.4573           | ng    | 99       |
| T Trichlorofluoromethane           | 2.145                | 101.0 | 555477  | 371.4290           | ng    | 98       |
| T 1,1-Dichloroethene               | 2.700                | 96.0  | 322557  | 380.3725           | ng    | 100      |
| T Methylene chloride               | 3.330                | 49.0  | 435116  | 348.0666           | ng    | 99       |
| T trans-1,2-Dichloroethene         | 3.715                | 96.0  | 325415  | 376.1367           | ng    | 97       |
| T Methyl tert-butyl ether (MTBE)   | 3.751                | 73.0  | 437439  | 391.1767           | ng    | 100      |
| T 1,1-Dichloroethane               | 4.381                | 63.0  | 612660  | 380.4437           | ng    | 99       |
| T 2,2-Dichloropropane              | 5.190                | 77.0  | 446282  | 369.8436           | ng    | 100      |
| T cis-1,2-Dichloroethene           | 5.212                | 96.0  | 339211  | 386.7236           | ng    | 97       |
| T Methyl ethyl ketone              | 5.279                | 43.0  | 470653  | 3961.3410          | ng    | 100      |
| T Bromochloromethane               | 5.516                | 128.0 | 135103  | 371.8004           | ng    | 99       |
| T Chloroform                       | 5.650                | 83.0  | 588080  | 366.9389           | ng    | 99       |













# Quantitation Results Report (QT Reviewed)

| Compound                    | RT     | QIon  | Resp.   | Conc.    | Units | Dev(Min) |
|-----------------------------|--------|-------|---------|----------|-------|----------|
| T 1,1,1-Trichloroethane     | 5.831  | 97.0  | 580748  | 386.6625 | ng    | 99       |
| T Carbon tetrachloride      | 6.024  | 117.0 | 572545  | 386.9014 | ng    | 99       |
| T 1,1-Dichloropropene       | 6.040  | 75.0  | 507157  | 397.1322 | ng    | 100      |
| T Benzene                   | 6.278  | 78.0  | 1293370 | 385.8526 | ng    | 99       |
| T 1,2-Dichloroethane        | 6.322  | 62.0  | 332775  | 366.9787 | ng    | 97       |
| T Trichloroethene           | 7.028  | 95.0  | 374370  | 394.4896 | ng    | 99       |
| T 1,2-Dichloropropane       | 7.270  | 63.0  | 324602  | 388.8502 | ng    | 98       |
| T Dibromomethane            | 7.396  | 93.0  | 134282  | 380.6547 | ng    | 96       |
| T Bromodichloromethane      | 7.585  | 83.0  | 375983  | 386.1940 | ng    | 100      |
| T cis-1,3-Dichloropropene   | 8.057  | 75.0  | 441168  | 400.7930 | ng    | 99       |
| T Toluene                   | 8.388  | 92.0  | 813204  | 397.0106 | ng    | 100      |
| T trans-1,3-Dichloropropene | 8.639  | 75.0  | 315063  | 402.1098 | ng    | 99       |
| T 1,1,2-Trichloroethane     | 8.818  | 83.0  | 152331  | 373.2534 | ng    | 100      |
| T Tetrachloroethene         | 8.938  | 163.8 | 319950  | 382.8796 | ng    | 99       |
| T 1,3-Dichloropropane       | 8.980  | 76.0  | 312547  | 389.3442 | ng    | 99       |
| T Chlorodibromomethane      | 9.203  | 129.0 | 247279  | 387.6812 | ng    | 99       |
| T 1,2-Dibromoethane         | 9.306  | 107.0 | 168577  | 377.7698 | ng    | 100      |
| T Chlorobenzene             | 9.802  | 112.0 | 867732  | 386.9455 | ng    | 100      |
| T 1,1,1,2-Tetrachloroethane | 9.892  | 131.0 | 307436  | 392.1859 | ng    | 96       |
| T Ethylbenzene              | 9.919  | 91.0  | 1574219 | 404.7587 | ng    | 100      |
| T m+p-Xylenes               | 10.039 | 106.0 | 1228570 | 812.8556 | ng    | 100      |
| T o-Xylene                  | 10.433 | 106.0 | 549244  | 408.2043 | ng    | 100      |
| T Styrene                   | 10.447 | 104.0 | 896331  | 413.7595 | ng    | 99       |
| T Bromoform                 | 10.628 | 172.5 | 129038  | 378.2200 | ng    | 99       |
| T Bromobenzene              | 11.093 | 156.0 | 333431  | 386.4420 | ng    | 98       |
| T 1,1,2,2-Tetrachloroethane | 11.110 | 83.0  | 182470  | 367.4276 | ng    | 98       |
| T 1,2,3-Trichloropropane    | 11.149 | 110.0 | 48325   | 363.6732 | ng    | 100      |
| T 2-Chlorotoluene           | 11.291 | 126.0 | 336386  | 391.8269 | ng    | 98       |
| T 4-Chlorotoluene           | 11.400 | 91.0  | 1109221 | 396.2756 | ng    | 100      |
| T 1,3-Dichlorobenzene       | 12.033 | 146.0 | 603674  | 383.6225 | ng    | 100      |
| T 1,4-Dichlorobenzene       | 12.125 | 146.0 | 595919  | 371.3969 | ng    | 98       |
| T 1,2-Dichlorobenzene       | 12.493 | 146.0 | 499147  | 375.3283 | ng    | 99       |

(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (\*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak




# Quantitation Results Report (QT Reviewed)

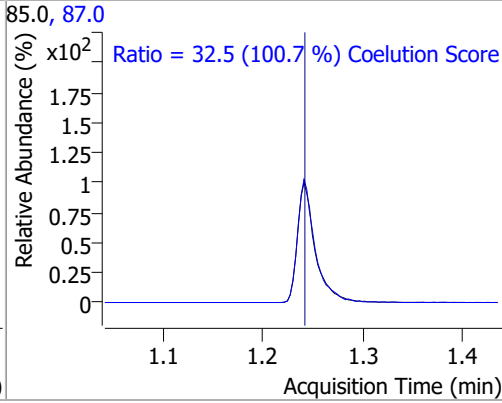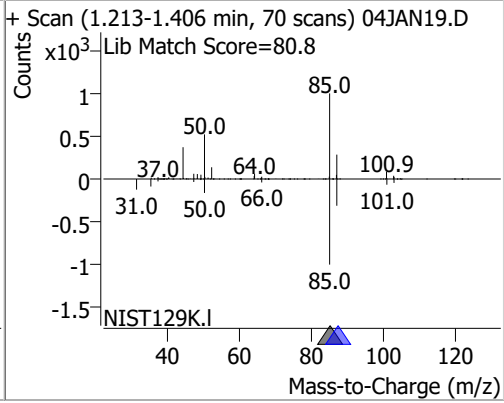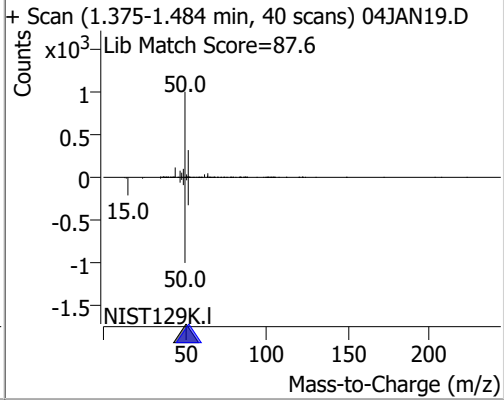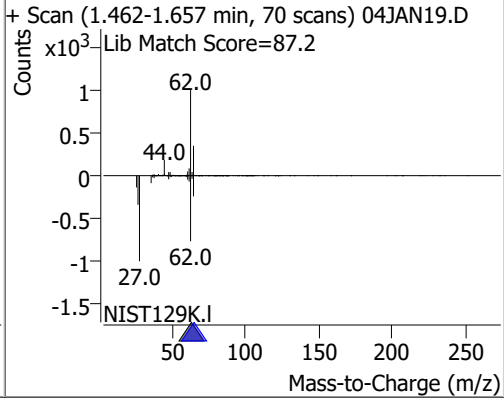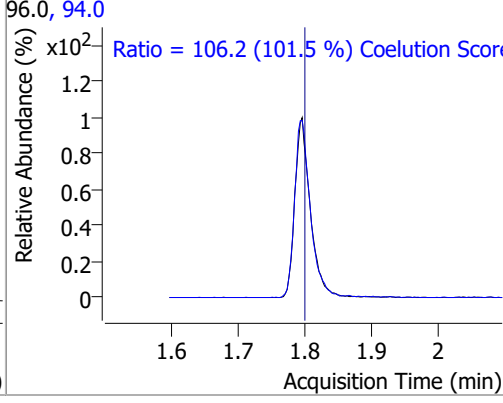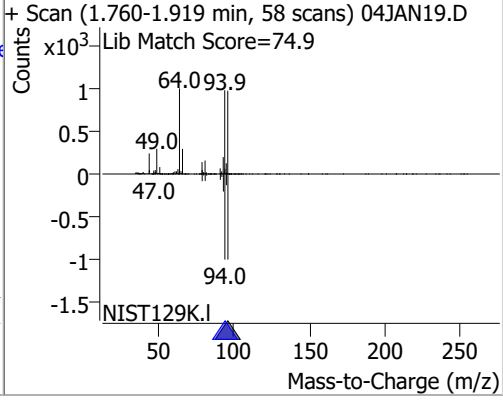
| Compound                                                                           | Conc.                                                                                | RT   | Dev(Min)                                                                              | Resp.  | QIon | QRatio                                       | Lower | Upper |
|------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------|------|---------------------------------------------------------------------------------------|--------|------|----------------------------------------------|-------|-------|
| Dichlorodifluoromethane                                                            | 373.9449                                                                             | 1.24 | 0.00                                                                                  | 412544 | 87.0 | 32.5                                         | 2.3   | 62.3  |
| + EIC (85.0) Scan 04JAN19.D                                                        |                                                                                      |      | 85.0, 87.0                                                                            |        |      | + Scan (1.213-1.406 min, 70 scans) 04JAN19.D |       |       |
|    |    |      |    |        |      |                                              |       |       |
| Chloromethane                                                                      | 352.0836                                                                             | 1.41 | 0.00                                                                                  | 471454 | 52.0 | 32.6                                         | 2.1   | 62.1  |
| + EIC (50.0) Scan 04JAN19.D                                                        |                                                                                      |      | 50.0, 52.0                                                                            |        |      | + Scan (1.375-1.484 min, 40 scans) 04JAN19.D |       |       |
|   |   |      |   |        |      |                                              |       |       |
| Vinyl chloride                                                                     | 372.3564                                                                             | 1.50 | 0.00                                                                                  | 448643 | 64.0 | 32.8                                         | 0.0   | 59.9  |
| + EIC (62.0) Scan 04JAN19.D                                                        |                                                                                      |      | 62.0, 64.0                                                                            |        |      | + Scan (1.462-1.657 min, 70 scans) 04JAN19.D |       |       |
|  |  |      |  |        |      |                                              |       |       |
| Bromomethane                                                                       | 385.1259                                                                             | 1.80 | 0.00                                                                                  | 207491 | 94.0 | 106.2                                        | 74.6  | 134.6 |
| + EIC (96.0) Scan 04JAN19.D                                                        |                                                                                      |      | 96.0, 94.0                                                                            |        |      | + Scan (1.760-1.919 min, 58 scans) 04JAN19.D |       |       |
|  |  |      |  |        |      |                                              |       |       |

# Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|-------|----|----------|-------|------|--------|-------|-------|
|----------|-------|----|----------|-------|------|--------|-------|-------|




| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|-------|----|----------|-------|------|--------|-------|-------|
|----------|-------|----|----------|-------|------|--------|-------|-------|

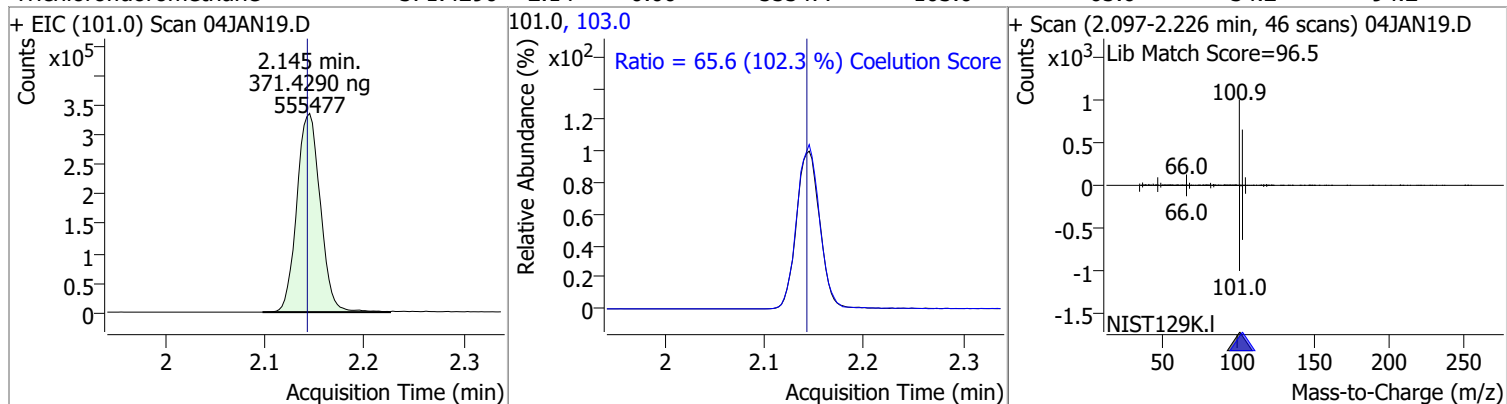

| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|-------|----|----------|-------|------|--------|-------|-------|
|----------|-------|----|----------|-------|------|--------|-------|-------|

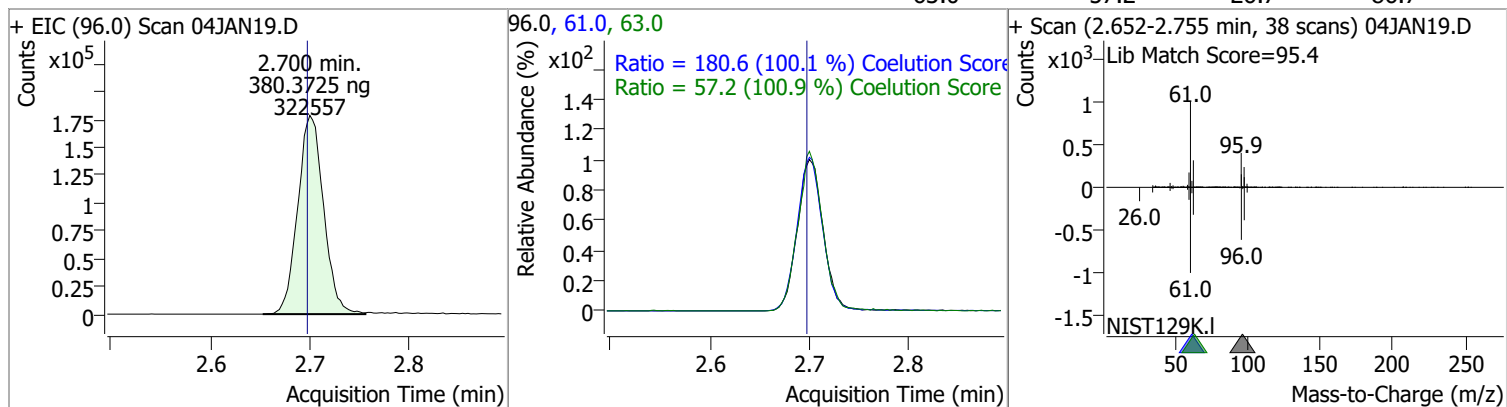


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|-------|----|----------|-------|------|--------|-------|-------|
|----------|-------|----|----------|-------|------|--------|-------|-------|




# Quantitation Results Report (QT Reviewed)


| Compound                 | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------------|----------|------|----------|--------|------|--------|-------|-------|
| trans-1,2-Dichloroethene | 376.1367 | 3.71 | 0.00     | 325415 | 61.0 | 158.9  | 123.9 | 183.9 |
|                          |          |      |          |        | 98.0 | 63.7   | 35.7  | 95.7  |

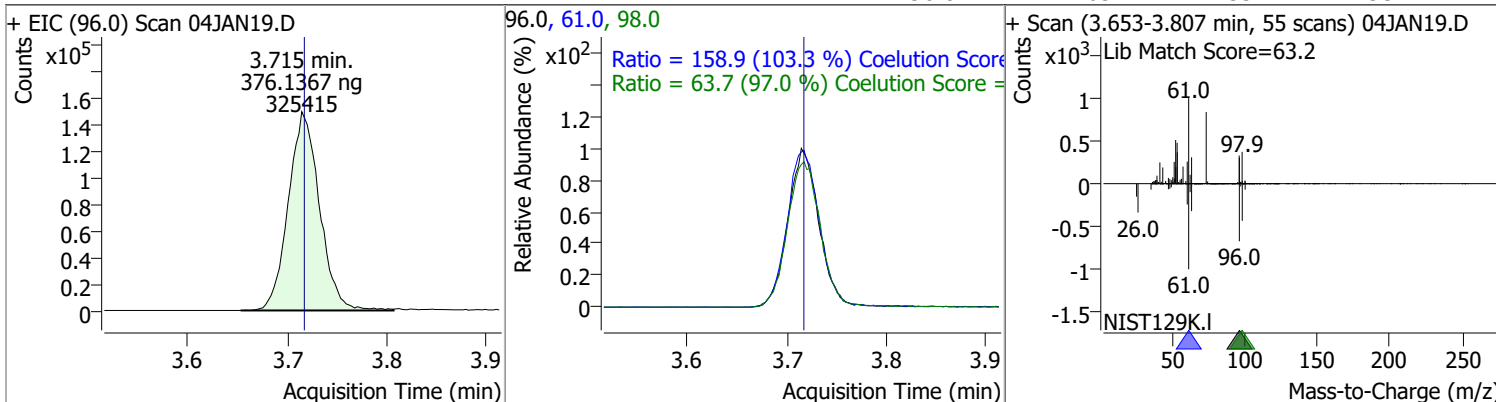

| Compound                       | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------------------|----------|------|----------|--------|------|--------|-------|-------|
| Methyl tert-butyl ether (MTBE) | 391.1767 | 3.75 | 0.00     | 437439 | 57.0 | 24.4   | 0.0   | 54.6  |

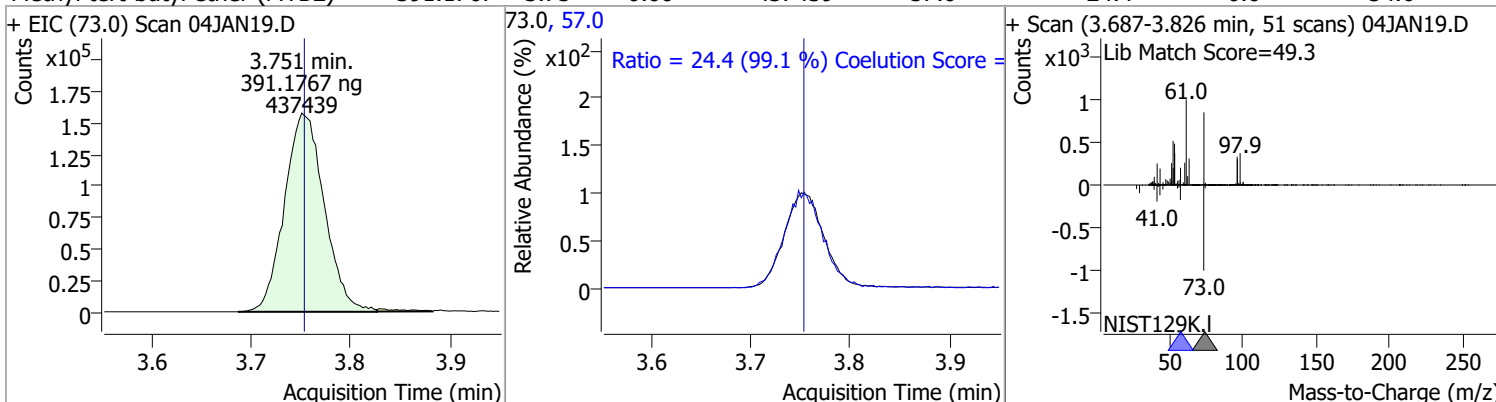


| Compound           | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1-Dichloroethane | 380.4437 | 4.38 | 0.00     | 612660 | 65.0 | 31.4   | 2.1   | 62.1  |
|                    |          |      |          |        | 83.0 | 13.1   | 0.0   | 43.7  |

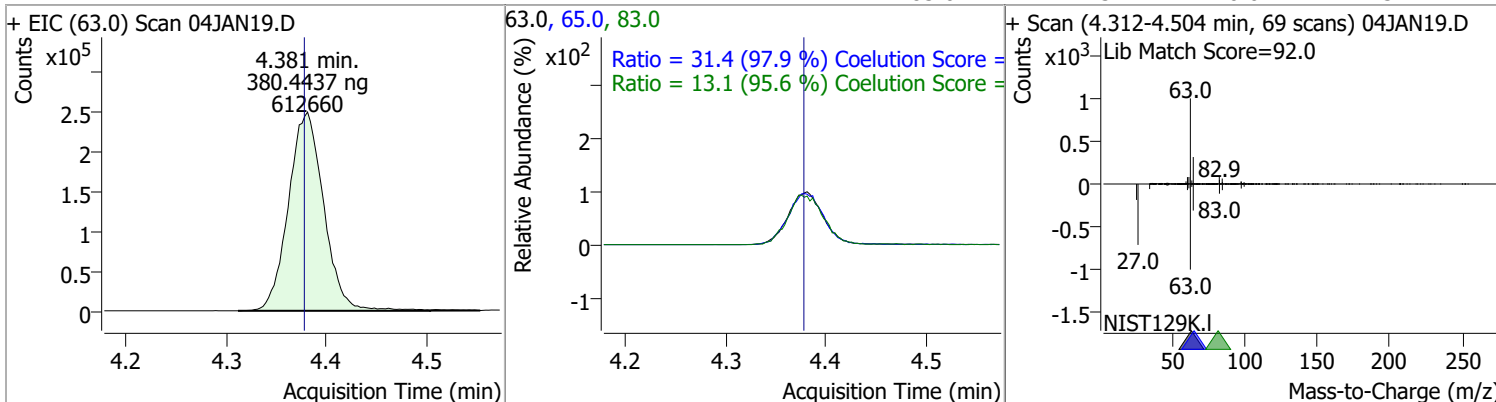


# Quantitation Results Report (QT Reviewed)


| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 2,2-Dichloropropane | 369.8436 | 5.19 | -0.01    | 446282 | 41.0 | 66.5   | 36.5  | 96.5  |
|                     |          |      |          |        | 97.0 | 23.5   | 0.0   | 53.2  |




| Compound               | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,2-Dichloroethene | 386.7236 | 5.21 | 0.00     | 339211 | 61.0 | 162.9  | 137.2 | 197.2 |
|                        |          |      |          |        | 98.0 | 64.4   | 37.3  | 97.3  |



| Compound            | Conc.     | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|-----------|------|----------|--------|------|--------|-------|-------|
| Methyl ethyl ketone | 3961.3410 | 5.28 | 0.00     | 470653 | 72.0 | 21.5   | 0.0   | 51.3  |

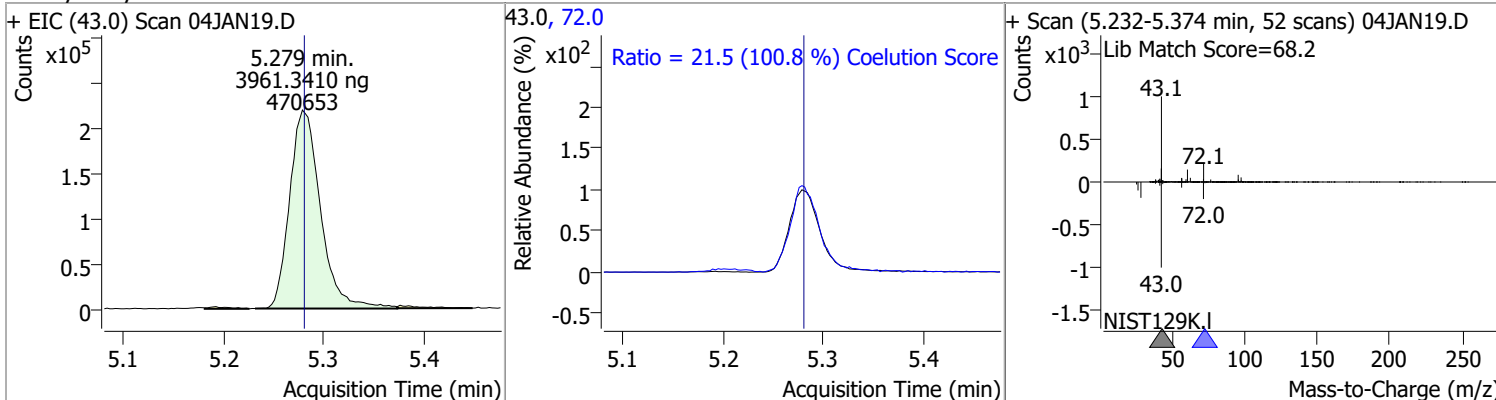


| Compound           | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| Bromochloromethane | 371.8004 | 5.52 | 0.00     | 135103 | 49.0 | 184.8  | 152.9 | 212.9 |

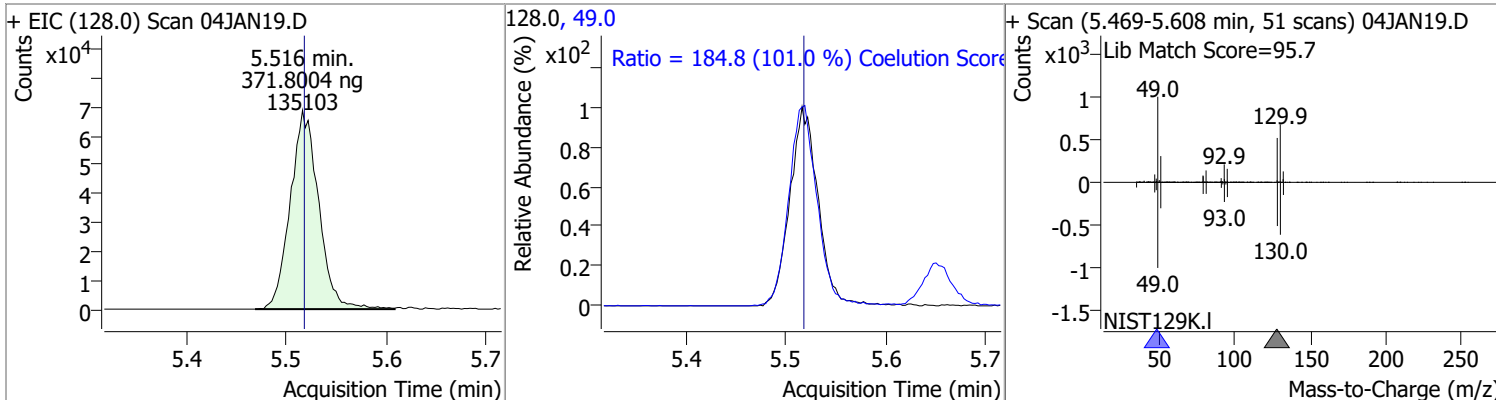


# Quantitation Results Report (QT Reviewed)


| Compound   | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|------|--------|-------|-------|
| Chloroform | 366.9389 | 5.65 | 0.00     | 588080 | 85.0 | 65.5   | 36.0  | 96.0  |




| Compound              | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1,1-Trichloroethane | 386.6625 | 5.83 | 0.00     | 580748 | 99.0 | 64.2   | 34.7  | 94.7  |
|                       |          |      |          |        | 61.0 | 47.7   | 18.1  | 78.1  |



| Compound             | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Dibromofluoromethane | 384.7503 | 5.85 | 0.00     | 305158 | 191.5 | 22.0   | 0.0   | 53.1  |




| Compound             | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Carbon tetrachloride | 386.9014 | 6.02 | 0.00     | 572545 | 119.0 | 96.4   | 67.2  | 127.2 |
|                      |          |      |          |        | 121.0 | 30.6   | 0.1   | 60.1  |

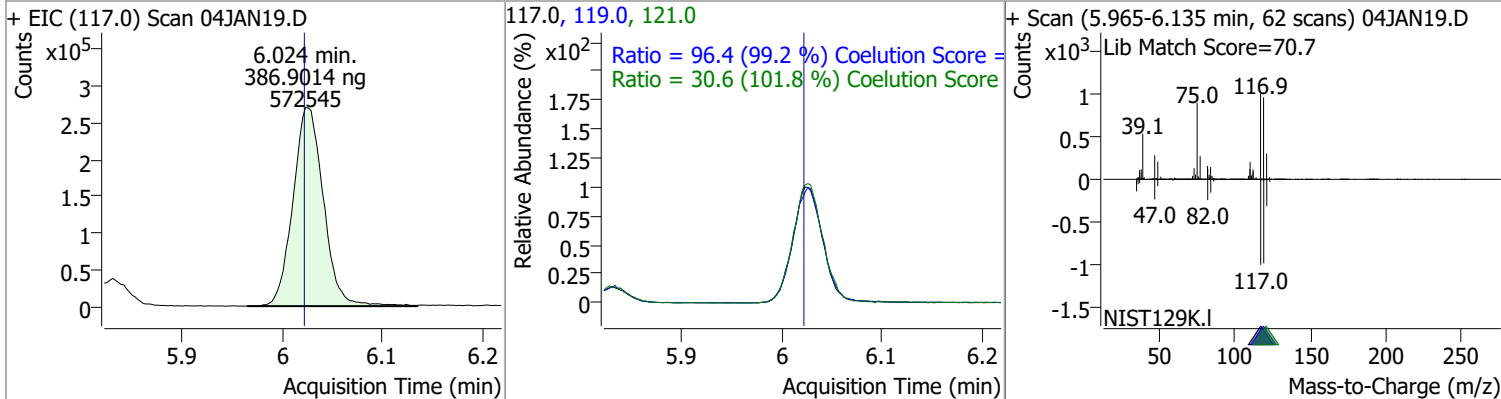


# Quantitation Results Report (QT Reviewed)


| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|-------|--------|-------|-------|
| 1,1-Dichloropropene | 397.1322 | 6.04 | 0.00     | 507157 | 110.0 | 36.0   | 5.9   | 65.9  |
|                     |          |      |          |        | 77.0  | 30.5   | 0.1   | 60.1  |




| Compound              | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 378.3335 | 6.23 | 0.00     | 129608 | 65.0 | 196.4  | 166.5 | 226.5 |



| Compound | Conc.    | RT   | Dev(Min) | Resp.   | QIon | QRatio | Lower | Upper |
|----------|----------|------|----------|---------|------|--------|-------|-------|
| Benzene  | 385.8526 | 6.28 | 0.00     | 1293370 | 77.0 | 23.3   | 0.0   | 53.5  |




| Compound           | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloroethane | 366.9787 | 6.32 | 0.00     | 332775 | 64.0 | 31.9   | 0.0   | 59.9  |
|                    |          |      |          |        | 98.0 | 7.9    | 0.0   | 37.6  |




# Quantitation Results Report (QT Reviewed)


| Compound        | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|-----------------|----------|------|----------|--------|-------|--------|-------|-------|
| Trichloroethene | 394.4896 | 7.03 | 0.00     | 374370 | 130.0 | 102.7  | 71.5  | 131.5 |
|                 |          |      |          |        | 97.0  | 64.4   | 34.1  | 94.1  |

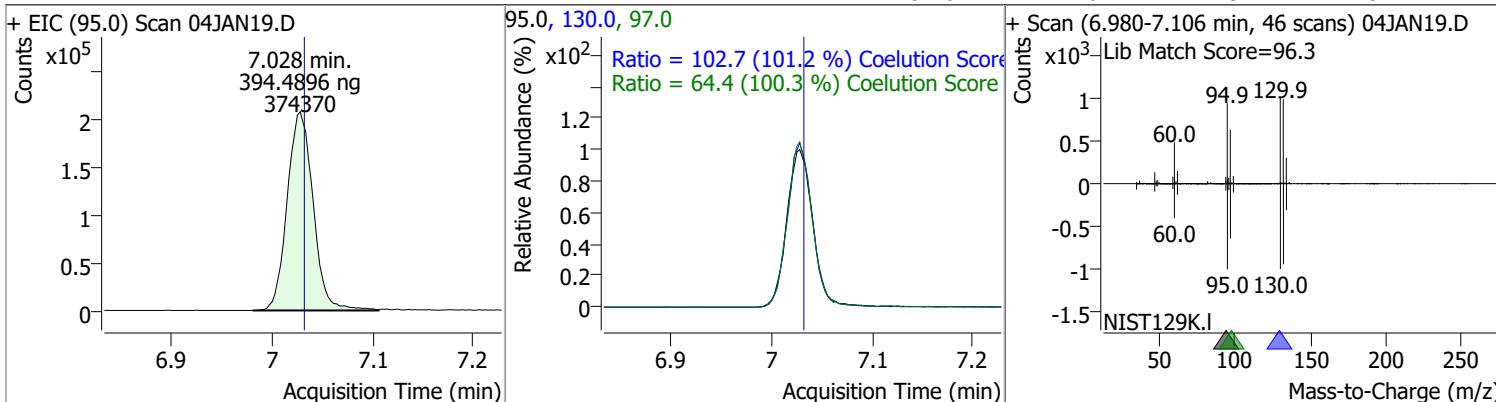

| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloropropane | 388.8502 | 7.27 | 0.00     | 324602 | 76.0 | 39.1   | 8.2   | 68.2  |

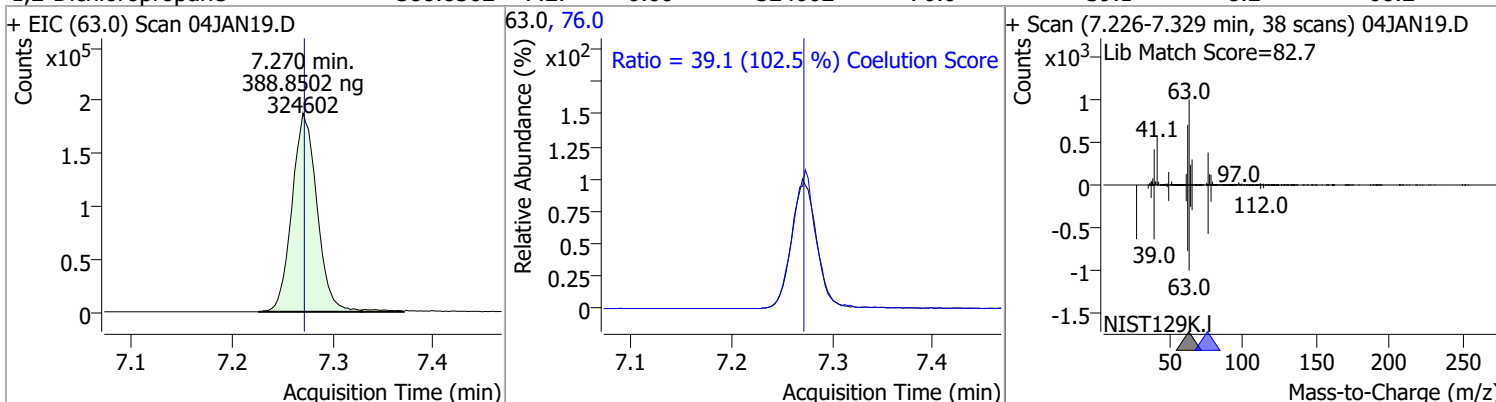


| Compound       | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------|----------|------|----------|--------|-------|--------|-------|-------|
| Dibromomethane | 380.6547 | 7.40 | 0.00     | 134282 | 173.5 | 107.8  | 83.7  | 143.7 |
|                |          |      |          |        | 95.0  | 83.6   | 52.2  | 112.2 |

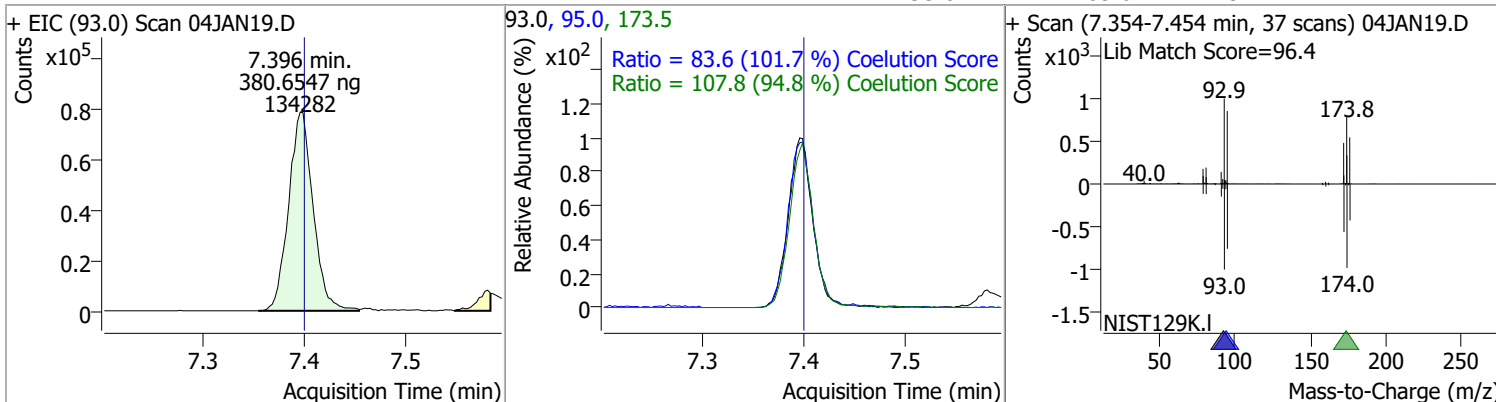


# Quantitation Results Report (QT Reviewed)


| Compound             | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Bromodichloromethane | 386.1940 | 7.59 | 0.00     | 375983 | 85.0  | 64.5   | 34.5  | 94.5  |
|                      |          |      |          |        | 127.0 | 9.2    | 0.0   | 39.6  |

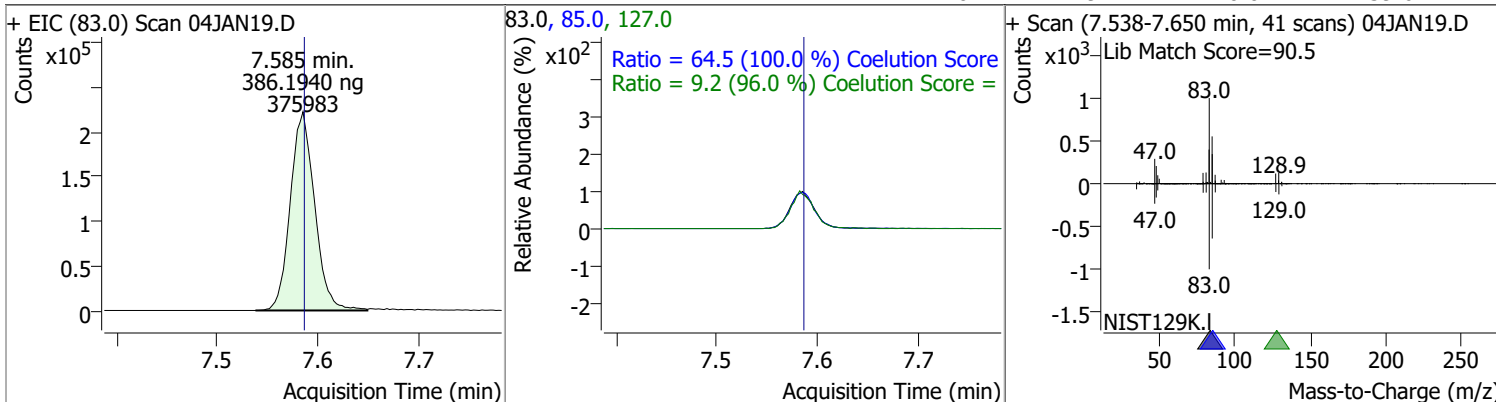

| Compound                | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|-------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,3-Dichloropropene | 400.7930 | 8.06 | 0.00     | 441168 | 39.0 | 52.9   | 23.3  | 83.3  |
|                         |          |      |          |        | 77.0 | 31.8   | 1.0   | 61.0  |

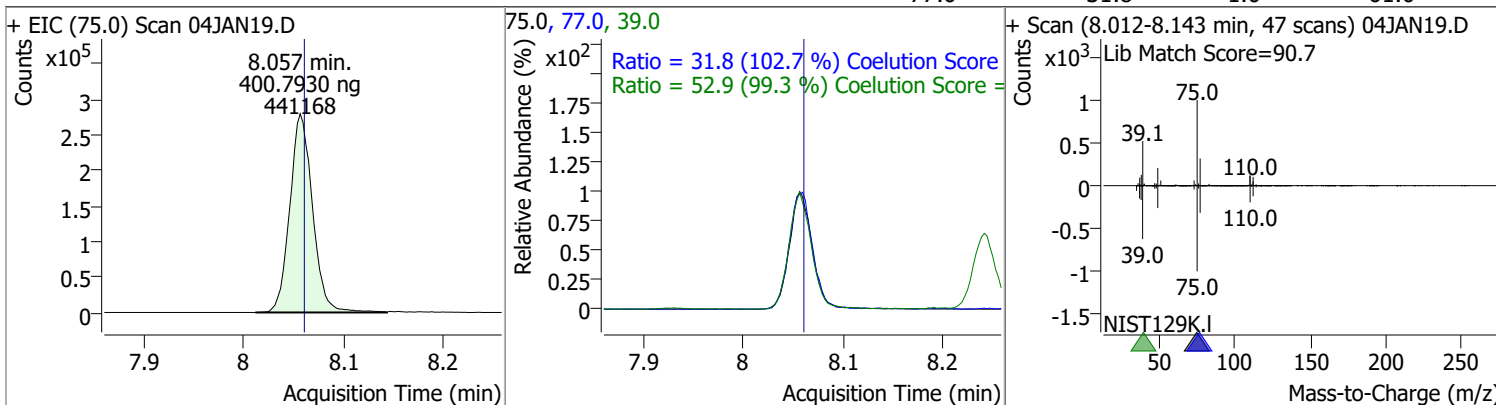


| Compound   | Conc.    | RT   | Dev(Min) | Resp.   | QIon  | QRatio | Lower | Upper |
|------------|----------|------|----------|---------|-------|--------|-------|-------|
| Toluene-d8 | 405.5583 | 8.32 | 0.00     | 1229775 | 100.0 | 64.2   | 34.4  | 94.4  |
|            |          |      |          |         | 99.0  | 9.4    | 0.0   | 39.6  |

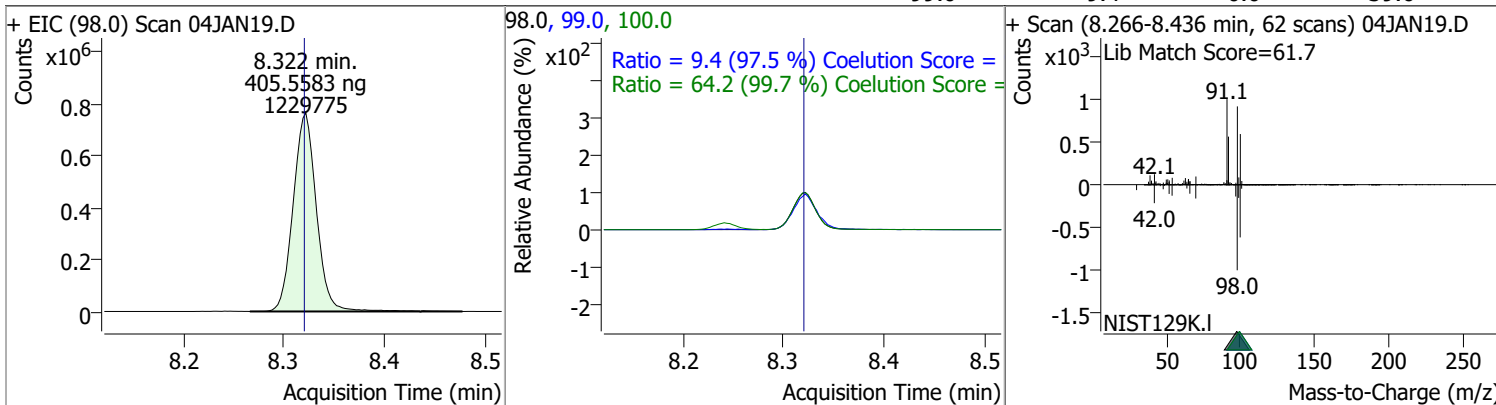




# Quantitation Results Report (QT Reviewed)


| Compound | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|----------|----------|------|----------|--------|------|--------|-------|-------|
| Toluene  | 397.0106 | 8.39 | 0.00     | 813204 | 91.0 | 175.4  | 145.8 | 205.8 |



| Compound                  | Conc.    | RT   | Dev(Min) | Resp.  | QIon         | QRatio       | Lower       | Upper        |
|---------------------------|----------|------|----------|--------|--------------|--------------|-------------|--------------|
| trans-1,3-Dichloropropene | 402.1098 | 8.64 | 0.00     | 315063 | 39.0<br>77.0 | 52.3<br>32.6 | 23.4<br>2.4 | 83.4<br>62.4 |




| Compound              | Conc.    | RT   | Dev(Min) | Resp.  | QIon         | QRatio        | Lower        | Upper         |
|-----------------------|----------|------|----------|--------|--------------|---------------|--------------|---------------|
| 1,1,2-Trichloroethane | 373.2534 | 8.82 | 0.00     | 152331 | 97.0<br>85.0 | 114.6<br>66.7 | 84.6<br>37.6 | 144.6<br>97.6 |




# Quantitation Results Report (QT Reviewed)


| Compound          | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|-------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Tetrachloroethene | 382.8796 | 8.94 | 0.00     | 319950 | 165.8 | 130.7  | 98.6  | 158.6 |
|                   |          |      |          |        | 129.0 | 91.3   | 61.5  | 121.5 |

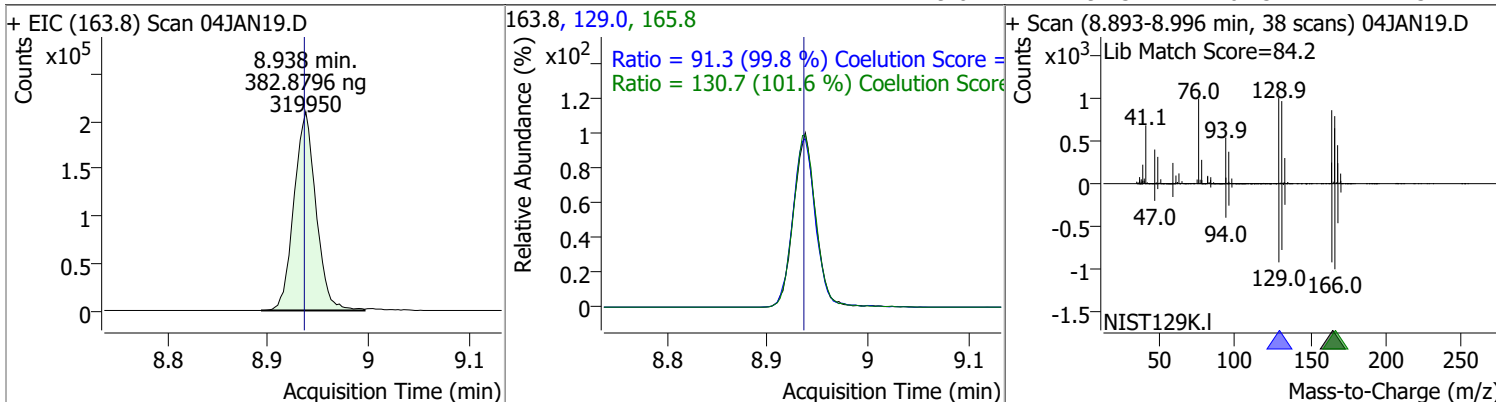


| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,3-Dichloropropane | 389.3442 | 8.98 | 0.00     | 312547 | 78.0 | 32.2   | 2.9   | 62.9  |

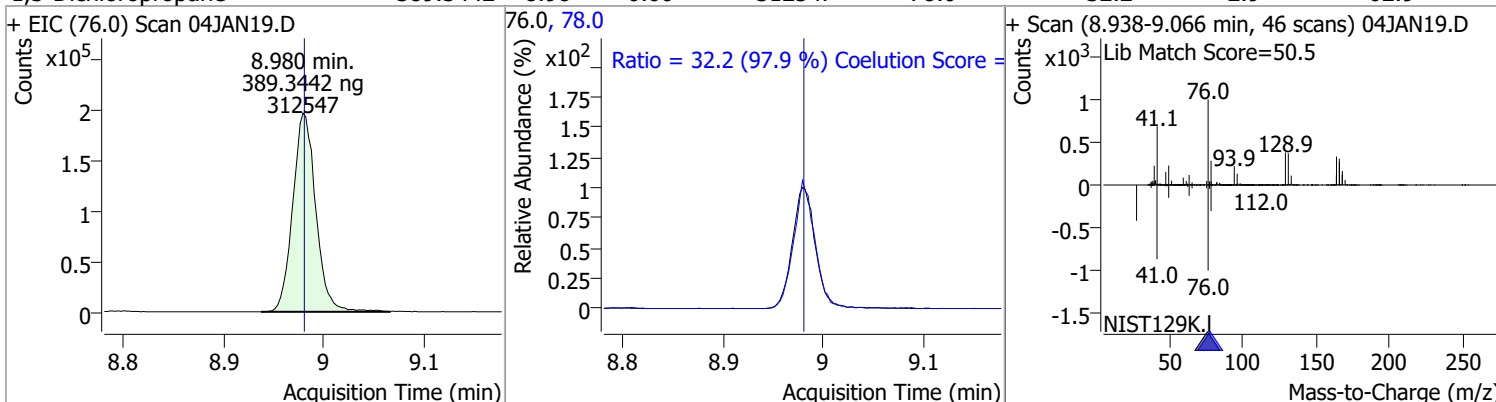

| Compound             | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Chlorodibromomethane | 387.6812 | 9.20 | 0.00     | 247279 | 127.0 | 77.1   | 48.0  | 108.0 |

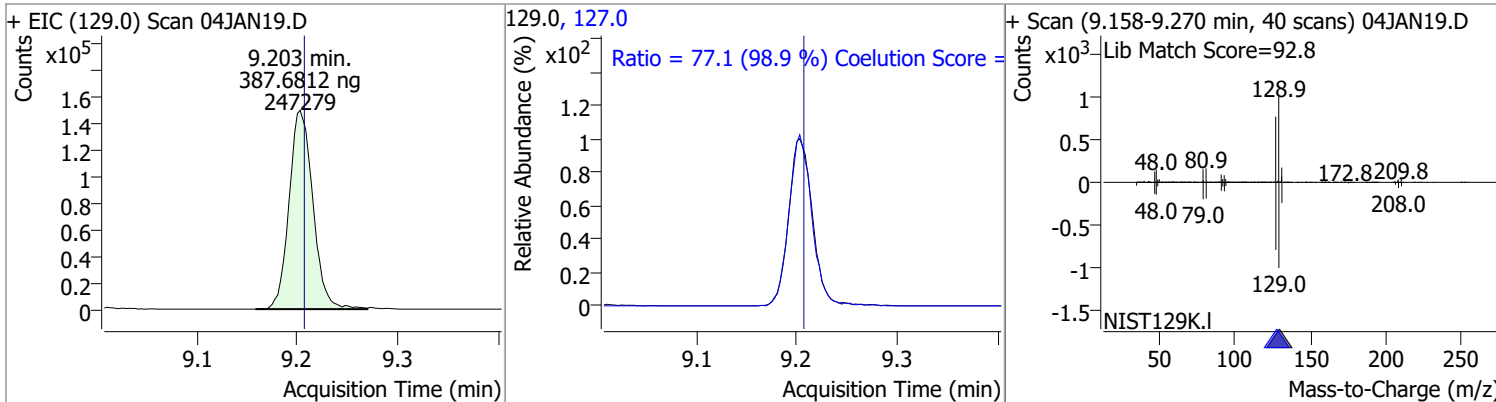

| Compound          | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|-------------------|----------|------|----------|--------|-------|--------|-------|-------|
| 1,2-Dibromoethane | 377.7698 | 9.31 | 0.00     | 168577 | 109.0 | 94.6   | 64.5  | 124.5 |

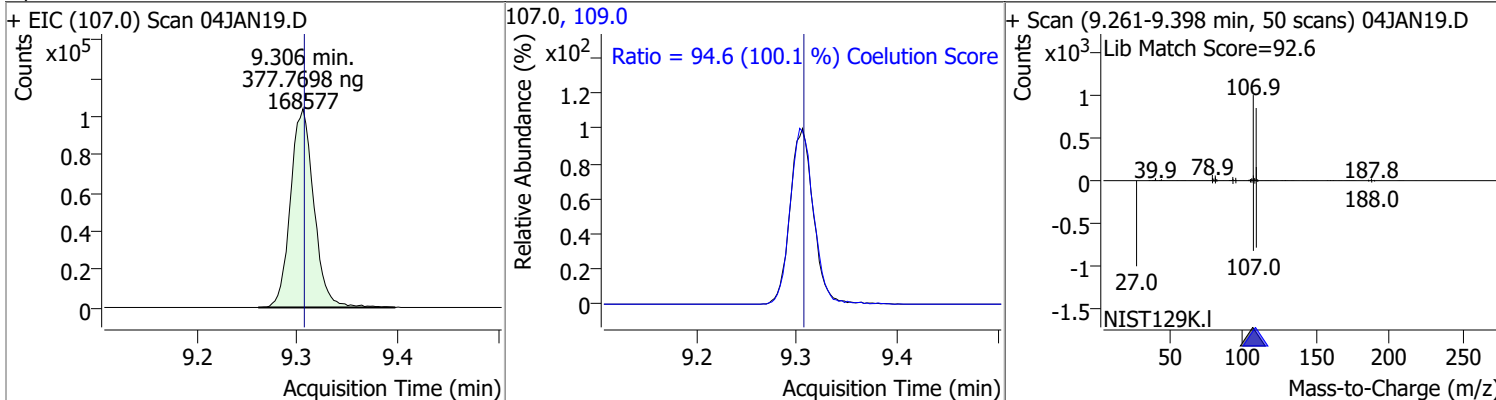


# Quantitation Results Report (QT Reviewed)


| Compound                     | Conc.    | RT    | Dev(Min)     | Resp.   | QIon  | QRatio                                        | Lower | Upper |
|------------------------------|----------|-------|--------------|---------|-------|-----------------------------------------------|-------|-------|
| Chlorobenzene                | 386.9455 | 9.80  | 0.00         | 867732  | 114.0 | 32.3                                          | 2.1   | 62.1  |
| + EIC (112.0) Scan 04JAN19.D |          |       | 112.0, 114.0 |         |       | + Scan (9.758-9.889 min, 48 scans) 04JAN19.D  |       |       |
|                              |          |       |              |         |       |                                               |       |       |
| 1,1,1,2-Tetrachloroethane    | 392.1859 | 9.89  | 0.00         | 307436  | 133.0 | 94.2                                          | 68.6  | 128.6 |
| + EIC (131.0) Scan 04JAN19.D |          |       | 131.0, 133.0 |         |       | + Scan (9.847-9.953 min, 39 scans) 04JAN19.D  |       |       |
|                              |          |       |              |         |       |                                               |       |       |
| Ethylbenzene                 | 404.7587 | 9.92  | 0.00         | 1574219 | 106.0 | 31.1                                          | 1.1   | 61.1  |
| + EIC (91.0) Scan 04JAN19.D  |          |       | 91.0, 106.0  |         |       | + Scan (9.872-9.995 min, 45 scans) 04JAN19.D  |       |       |
|                              |          |       |              |         |       |                                               |       |       |
| m+p-Xylenes                  | 812.8556 | 10.04 | 0.00         | 1228570 | 91.0  | 201.2                                         | 171.4 | 231.4 |
| + EIC (106.0) Scan 04JAN19.D |          |       | 106.0, 91.0  |         |       | + Scan (9.995-10.109 min, 42 scans) 04JAN19.D |       |       |
|                              |          |       |              |         |       |                                               |       |       |

# Quantitation Results Report (QT Reviewed)


| Compound | Conc.    | RT    | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|----------|----------|-------|----------|--------|------|--------|-------|-------|
| o-Xylene | 408.2043 | 10.43 | 0.00     | 549244 | 91.0 | 213.2  | 183.1 | 243.1 |




| Compound | Conc.    | RT    | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|----------|----------|-------|----------|--------|------|--------|-------|-------|
| Styrene  | 413.7595 | 10.45 | 0.00     | 896331 | 78.0 | 50.0   | 19.6  | 79.6  |



| Compound  | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|-----------|----------|-------|----------|--------|-------|--------|-------|-------|
| Bromoform | 378.2200 | 10.63 | 0.00     | 129038 | 170.5 | 52.5   | 22.1  | 82.1  |
|           |          |       |          |        | 174.5 | 50.4   | 20.1  | 80.1  |

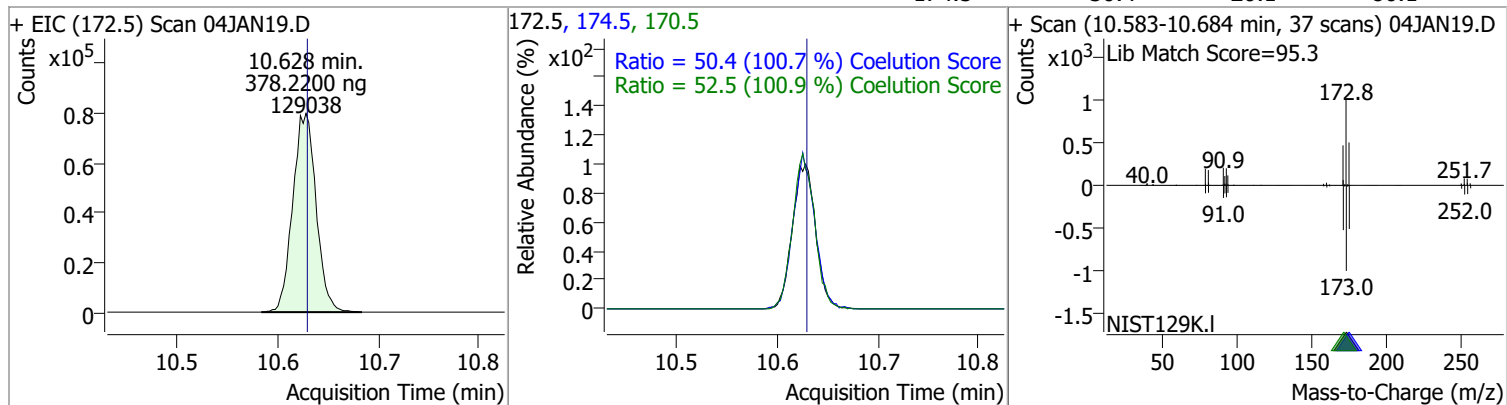


| Compound             | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 394.6566 | 10.95 | 0.00     | 385474 | 174.0 | 94.4   | 61.7  | 121.7 |
|                      |          |       |          |        | 176.0 | 92.3   | 60.6  | 120.6 |




# Quantitation Results Report (QT Reviewed)


| Compound     | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|--------------|----------|-------|----------|--------|-------|--------|-------|-------|
| Bromobenzene | 386.4420 | 11.09 | 0.00     | 333431 | 77.0  | 142.7  | 115.7 | 175.7 |
|              |          |       |          |        | 158.0 | 98.4   | 66.5  | 126.5 |




| Compound                  | Conc.    | RT    | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------------|----------|-------|----------|--------|------|--------|-------|-------|
| 1,1,2,2-Tetrachloroethane | 367.4276 | 11.11 | -0.01    | 182470 | 85.0 | 64.9   | 36.2  | 96.2  |
|                           |          |       |          |        | 83.0 | 77.0   | 155.9 | 130.9 |



| Compound               | Conc.    | RT    | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|------------------------|----------|-------|----------|-------|-------|--------|-------|-------|
| 1,2,3-Trichloropropane | 363.6732 | 11.15 | 0.00     | 48325 | 112.0 | 63.7   | 33.5  | 93.5  |
|                        |          |       |          |       | 110.0 | 75.0   | 157.9 | 109.9 |




| Compound        | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|-----------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 2-Chlorotoluene | 391.8269 | 11.29 | 0.00     | 336386 | 91.0  | 285.3  | 252.3 | 312.3 |
|                 |          |       |          |        | 126.0 | 126.0  | 91.0  | 63.0  |




# Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|-------|----|----------|-------|------|--------|-------|-------|
|----------|-------|----|----------|-------|------|--------|-------|-------|



|                 |          |       |      |         |       |      |     |      |
|-----------------|----------|-------|------|---------|-------|------|-----|------|
| 4-Chlorotoluene | 396.2756 | 11.40 | 0.00 | 1109221 | 126.0 | 31.5 | 1.7 | 61.7 |
|-----------------|----------|-------|------|---------|-------|------|-----|------|






|                     |          |       |      |        |       |      |      |      |
|---------------------|----------|-------|------|--------|-------|------|------|------|
| 1,3-Dichlorobenzene | 383.6225 | 12.03 | 0.00 | 603674 | 148.0 | 63.5 | 33.6 | 93.6 |
|---------------------|----------|-------|------|--------|-------|------|------|------|



|                     |          |       |      |        |       |      |      |      |
|---------------------|----------|-------|------|--------|-------|------|------|------|
| 1,4-Dichlorobenzene | 371.3969 | 12.13 | 0.00 | 595919 | 148.0 | 64.9 | 33.1 | 93.1 |
|---------------------|----------|-------|------|--------|-------|------|------|------|


# Quantitation Results Report (QT Reviewed)

| Compound            | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,2-Dichlorobenzene | 375.3283 | 12.49 | 0.00     | 499147 | 148.0 | 63.8   | 33.9  | 93.9  |
|                     |          |       |          |        | 111.0 | 40.2   | 11.0  | 71.0  |

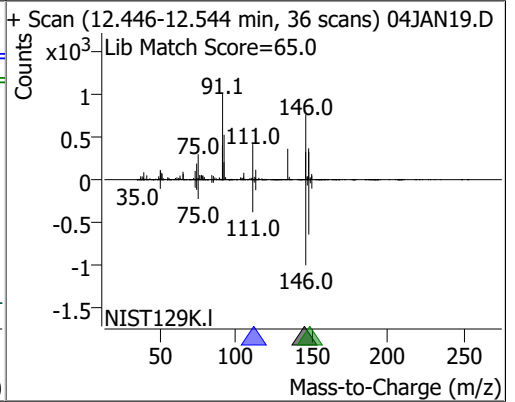

# Quantitation Results Report (QT Reviewed)

|                |                                     |                   |                       |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File      | 04JAN21.D                           | Operator          | MSC                   |
| Acq. Method    | 5975CACQF.M                         | Acq. Date-Time    | 1/4/2022 8:34:31 PM   |
| Sample Name    | ICAL010422_8                        | Instrument        | VOA5975C              |
| Vial           | 21                                  | Multiplier        | 1.00                  |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m  | Comment           |                       |
| Tune File      | BFB_Atune3.u                        | Tune Date         | 10/11/2021 4:02:00 PM |
| Batch Name     | VG010422_8260B.batch.bin            | Last Calib Update | 1/9/2022 8:59:52 PM   |
| Ref Library    | \\MASSHUNTER\Org\Library\NIST129K.I |                   |                       |

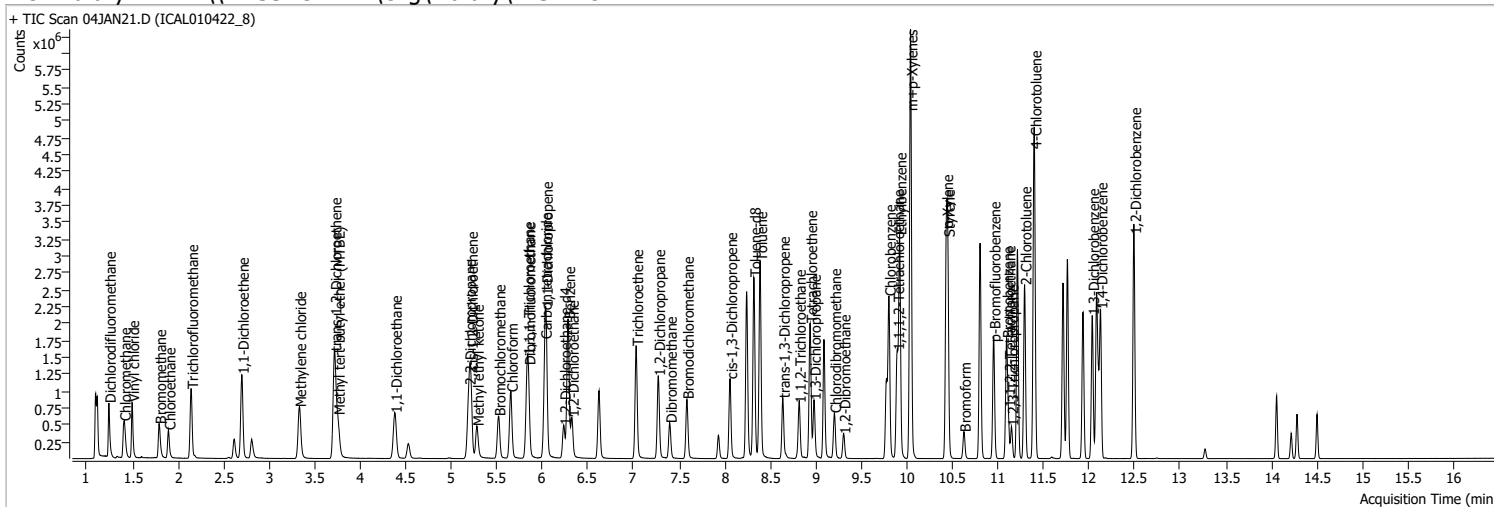

| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|----------|----|------|-------|-------|-------|----------|
|----------|----|------|-------|-------|-------|----------|

**Internal Standards**

|                          |        |       |        |          |    |        |
|--------------------------|--------|-------|--------|----------|----|--------|
| M Fluorobenzene          | 6.621  | 96.0  | 841364 | 250.0000 | ng | -0.003 |
| M Chlorobenzene-d5       | 9.774  | 82.0  | 313585 | 250.0000 | ng | 0.003  |
| M 1,4-Dichlorobenzene-d4 | 12.103 | 152.0 | 262971 | 250.0000 | ng | 0.003  |

**System Monitoring Compounds**

|                         |                      |       |         |                    |    |        |
|-------------------------|----------------------|-------|---------|--------------------|----|--------|
| S Dibromofluoromethane  | 5.845                | 113.0 | 404568  | 510.3991           | ng | 0.000  |
| Spiked Amount: 250.000  | Range: 80.0 - 119.0% |       |         | Recovery = 204.16% | *  |        |
| S 1,2-Dichloroethane-d4 | 6.233                | 67.0  | 174713  | 510.3080           | ng | 0.000  |
| Spiked Amount: 250.000  | Range: 81.0 - 118.0% |       |         | Recovery = 204.12% | *  |        |
| S Toluene-d8            | 8.319                | 98.0  | 1644540 | 544.2136           | ng | 0.000  |
| Spiked Amount: 250.000  | Range: 89.0 - 112.0% |       |         | Recovery = 217.69% | *  |        |
| S p-Bromofluorobenzene  | 10.949               | 95.0  | 521580  | 541.3964           | ng | -0.006 |
| Spiked Amount: 250.000  | Range: 85.0 - 114.0% |       |         | Recovery = 216.56% | *  |        |

**Target Compounds**

| Compound                         | RT    | QIon  | Resp.  | Conc.     | Units | QValue |
|----------------------------------|-------|-------|--------|-----------|-------|--------|
| T Dichlorodifluoromethane        | 1.241 | 85.0  | 545484 | 494.7474  | ng    | 99     |
| T Chloromethane                  | 1.406 | 50.0  | 642582 | 480.1747  | ng    | 100    |
| T Vinyl chloride                 | 1.495 | 62.0  | 600092 | 498.3563  | ng    | 95     |
| T Bromomethane                   | 1.793 | 96.0  | 277301 | 515.0141  | ng    | 98     |
| T Chloroethane                   | 1.894 | 64.0  | 287041 | 481.5143  | ng    | 98     |
| T Trichlorofluoromethane         | 2.145 | 101.0 | 731829 | 489.6475  | ng    | 99     |
| T 1,1-Dichloroethene             | 2.700 | 96.0  | 436507 | 515.0603  | ng    | 98     |
| T Methylene chloride             | 3.330 | 49.0  | 583438 | 466.9993  | ng    | 98     |
| T trans-1,2-Dichloroethene       | 3.718 | 96.0  | 440967 | 510.0097  | ng    | 98     |
| T Methyl tert-butyl ether (MTBE) | 3.754 | 73.0  | 584294 | 522.8187  | ng    | 99     |
| T 1,1-Dichloroethane             | 4.378 | 63.0  | 829359 | 515.3207  | ng    | 99     |
| T 2,2-Dichloropropane            | 5.190 | 77.0  | 601823 | 499.0473  | ng    | 98     |
| T cis-1,2-Dichloroethene         | 5.212 | 96.0  | 452377 | 516.0544  | ng    | 99     |
| T Methyl ethyl ketone            | 5.279 | 43.0  | 632539 | 5327.1253 | ng    | 99     |
| T Bromochloromethane             | 5.519 | 128.0 | 179618 | 494.6054  | ng    | 98     |
| T Chloroform                     | 5.653 | 83.0  | 783422 | 489.1221  | ng    | 99     |















# Quantitation Results Report (QT Reviewed)

| Compound                    | RT     | QIon  | Resp.   | Conc.     | Units | Dev(Min) |
|-----------------------------|--------|-------|---------|-----------|-------|----------|
| T 1,1,1-Trichloroethane     | 5.834  | 97.0  | 778785  | 518.8312  | ng    | 99       |
| T Carbon tetrachloride      | 6.024  | 117.0 | 770907  | 521.2630  | ng    | 98       |
| T 1,1-Dichloropropene       | 6.038  | 75.0  | 693669  | 543.5121  | ng    | 99       |
| T Benzene                   | 6.280  | 78.0  | 1714050 | 511.6658  | ng    | 100      |
| T 1,2-Dichloroethane        | 6.322  | 62.0  | 450739  | 497.3699  | ng    | 100      |
| T Trichloroethene           | 7.028  | 95.0  | 505400  | 534.4007  | ng    | 99       |
| T 1,2-Dichloropropane       | 7.270  | 63.0  | 436057  | 524.1695  | ng    | 100      |
| T Dibromomethane            | 7.396  | 93.0  | 176038  | 500.7456  | ng    | 98       |
| T Bromodichloromethane      | 7.585  | 83.0  | 502929  | 518.3718  | ng    | 100      |
| T cis-1,3-Dichloropropene   | 8.059  | 75.0  | 591147  | 538.9008  | ng    | 99       |
| T Toluene                   | 8.389  | 92.0  | 1095161 | 536.5101  | ng    | 99       |
| T trans-1,3-Dichloropropene | 8.637  | 75.0  | 416771  | 533.7551  | ng    | 99       |
| T 1,1,2-Trichloroethane     | 8.815  | 83.0  | 205463  | 505.1803  | ng    | 97       |
| T Tetrachloroethene         | 8.938  | 163.8 | 428812  | 514.9255  | ng    | 100      |
| T 1,3-Dichloropropane       | 8.980  | 76.0  | 408993  | 511.2479  | ng    | 100      |
| T Chlorodibromomethane      | 9.203  | 129.0 | 330813  | 520.4361  | ng    | 99       |
| T 1,2-Dibromoethane         | 9.303  | 107.0 | 225877  | 507.9234  | ng    | 99       |
| T Chlorobenzene             | 9.802  | 112.0 | 1153147 | 515.9957  | ng    | 100      |
| T 1,1,1,2-Tetrachloroethane | 9.892  | 131.0 | 406450  | 520.2855  | ng    | 98       |
| T Ethylbenzene              | 9.919  | 91.0  | 2111152 | 544.6881  | ng    | 100      |
| T m+p-Xylenes               | 10.039 | 106.0 | 1637879 | 1087.4082 | ng    | 99       |
| T o-Xylene                  | 10.430 | 106.0 | 734101  | 547.4764  | ng    | 100      |
| T Styrene                   | 10.449 | 104.0 | 1199879 | 555.7946  | ng    | 99       |
| T Bromoform                 | 10.625 | 172.5 | 175918  | 522.7660  | ng    | 98       |
| T Bromobenzene              | 11.094 | 156.0 | 439147  | 516.0104  | ng    | 98       |
| T 1,1,2,2-Tetrachloroethane | 11.113 | 83.0  | 240837  | 491.6700  | ng    | 99       |
| T 1,2,3-Trichloropropane    | 11.146 | 110.0 | 64422   | 491.5229  | ng    | 99       |
| T 2-Chlorotoluene           | 11.292 | 126.0 | 455991  | 538.4964  | ng    | 99       |
| T 4-Chlorotoluene           | 11.400 | 91.0  | 1468376 | 531.8471  | ng    | 100      |
| T 1,3-Dichlorobenzene       | 12.033 | 146.0 | 793993  | 511.5504  | ng    | 100      |
| T 1,4-Dichlorobenzene       | 12.125 | 146.0 | 794954  | 502.3001  | ng    | 99       |
| T 1,2-Dichlorobenzene       | 12.493 | 146.0 | 664247  | 506.3871  | ng    | 99       |


**(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (\*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak**

# Quantitation Results Report (QT Reviewed)

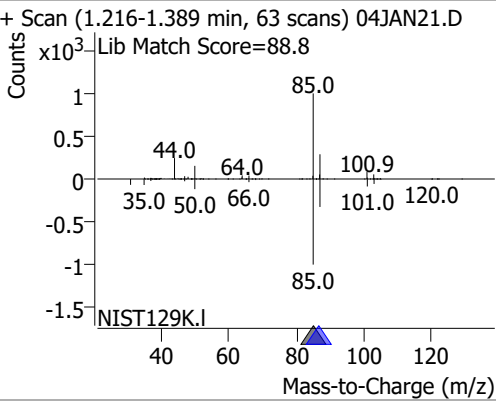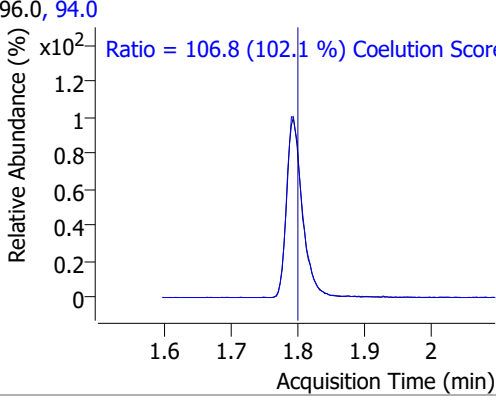
| Compound                                                                           | Conc.                               | RT   | Dev(Min)                                                                             | Resp.  | QIon | QRatio                                                                                | Lower | Upper |
|------------------------------------------------------------------------------------|-------------------------------------|------|--------------------------------------------------------------------------------------|--------|------|---------------------------------------------------------------------------------------|-------|-------|
| Dichlorodifluoromethane                                                            | 494.7474                            | 1.24 | 0.00                                                                                 | 545484 | 87.0 | 33.0                                                                                  | 2.3   | 62.3  |
| + EIC (85.0) Scan 04JAN21.D                                                        |                                     |      | 85.0, 87.0                                                                           |        |      | + Scan (1.216-1.389 min, 63 scans) 04JAN21.D                                          |       |       |
|    | 1.241 min.<br>494.7474 ng<br>545484 |      |    |        |      |    |       |       |
|                                                                                    |                                     |      | Ratio = 33.0 (102.4 %) Coelution Score                                               |        |      |                                                                                       |       |       |
| Chloromethane                                                                      | 480.1747                            | 1.41 | 0.00                                                                                 | 642582 | 52.0 | 32.1                                                                                  | 2.1   | 62.1  |
| + EIC (50.0) Scan 04JAN21.D                                                        |                                     |      | 50.0, 52.0                                                                           |        |      | + Scan (1.370-1.548 min, 65 scans) 04JAN21.D                                          |       |       |
|   | 1.406 min.<br>480.1747 ng<br>642582 |      |   |        |      |   |       |       |
|                                                                                    |                                     |      | Ratio = 32.1 (100.0 %) Coelution Score                                               |        |      |                                                                                       |       |       |
| Vinyl chloride                                                                     | 498.3563                            | 1.50 | 0.00                                                                                 | 600092 | 64.0 | 32.5                                                                                  | 0.0   | 59.9  |
| + EIC (62.0) Scan 04JAN21.D                                                        |                                     |      | 62.0, 64.0                                                                           |        |      | + Scan (1.464-1.679 min, 77 scans) 04JAN21.D                                          |       |       |
|  | 1.495 min.<br>498.3563 ng<br>600092 |      |  |        |      |  |       |       |
|                                                                                    |                                     |      | Ratio = 32.5 (108.8 %) Coelution Score                                               |        |      |                                                                                       |       |       |
| Bromomethane                                                                       | 515.0141                            | 1.79 | -0.01                                                                                | 277301 | 94.0 | 106.8                                                                                 | 74.6  | 134.6 |
| + EIC (96.0) Scan 04JAN21.D                                                        |                                     |      | 96.0, 94.0                                                                           |        |      | + Scan (1.757-1.941 min, 67 scans) 04JAN21.D                                          |       |       |
|  | 1.793 min.<br>515.0141 ng<br>277301 |      |  |        |      |  |       |       |
|                                                                                    |                                     |      | Ratio = 106.8 (102.1 %) Coelution Score                                              |        |      |                                                                                       |       |       |

# Quantitation Results Report (QT Reviewed)


| Compound     | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------|----------|------|----------|--------|------|--------|-------|-------|
| Chloroethane | 481.5143 | 1.89 | 0.00     | 287041 | 66.0 | 31.4   | 0.1   | 60.1  |




| Compound               | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|------------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Trichlorofluoromethane | 489.6475 | 2.14 | 0.00     | 731829 | 103.0 | 64.7   | 34.2  | 94.2  |



| Compound           | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1-Dichloroethene | 515.0603 | 2.70 | 0.00     | 436507 | 61.0 | 184.2  | 150.3 | 210.3 |
|                    |          |      |          |        | 63.0 | 57.2   | 26.7  | 86.7  |




| Compound           | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| Methylene chloride | 466.9993 | 3.33 | -0.01    | 583438 | 84.0 | 66.3   | 36.9  | 96.9  |
|                    |          |      |          |        | 86.0 | 42.3   | 14.3  | 74.3  |




# Quantitation Results Report (QT Reviewed)


| Compound                 | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------------|----------|------|----------|--------|------|--------|-------|-------|
| trans-1,2-Dichloroethene | 510.0097 | 3.72 | 0.00     | 440967 | 61.0 | 157.1  | 123.9 | 183.9 |
|                          |          |      |          |        | 98.0 | 64.1   | 35.7  | 95.7  |

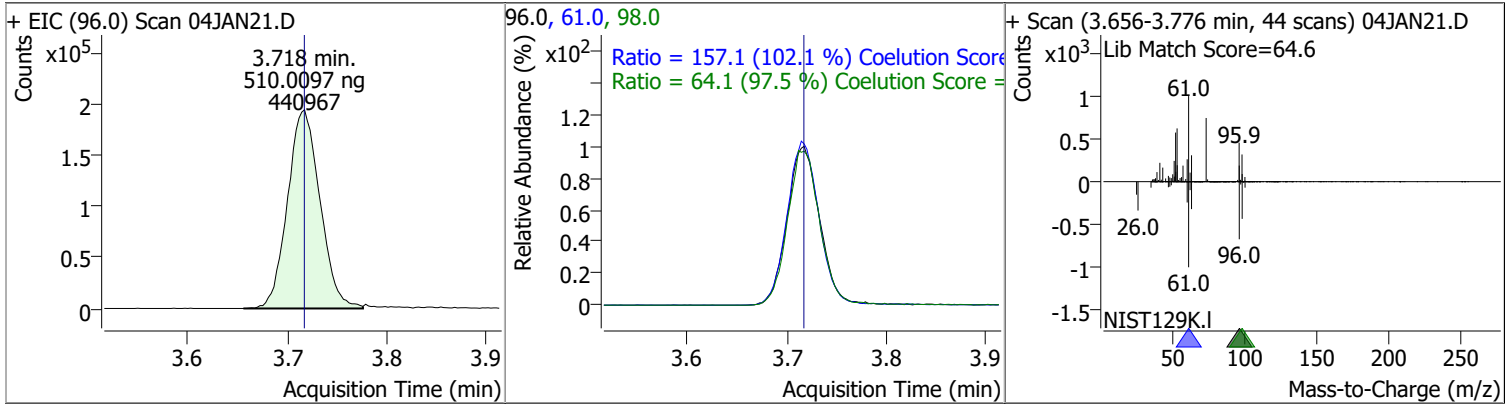

| Compound                       | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------------------|----------|------|----------|--------|------|--------|-------|-------|
| Methyl tert-butyl ether (MTBE) | 522.8187 | 3.75 | 0.00     | 584294 | 57.0 | 24.9   | 0.0   | 54.6  |

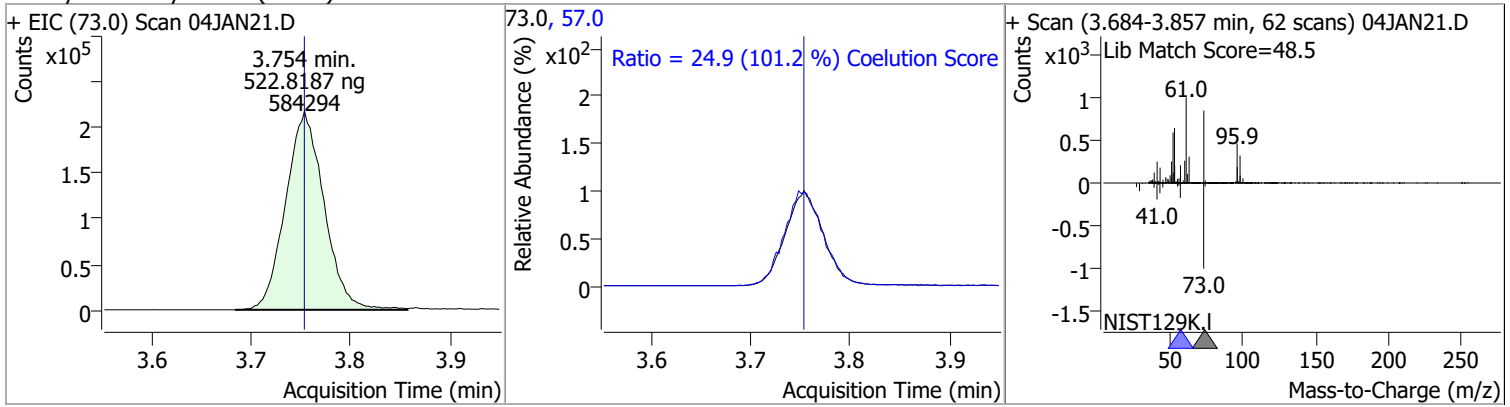


| Compound           | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1-Dichloroethane | 515.3207 | 4.38 | 0.00     | 829359 | 65.0 | 31.6   | 2.1   | 62.1  |
|                    |          |      |          |        | 83.0 | 12.8   | 0.0   | 43.7  |

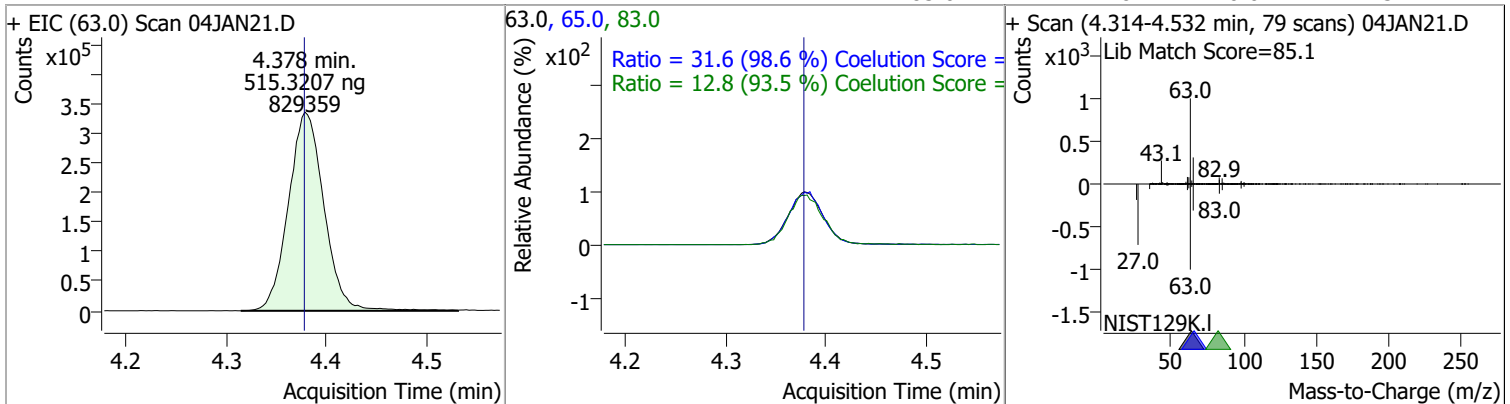


# Quantitation Results Report (QT Reviewed)


| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 2,2-Dichloropropane | 499.0473 | 5.19 | -0.01    | 601823 | 41.0 | 64.7   | 36.5  | 96.5  |
|                     |          |      |          |        | 97.0 | 22.9   | 0.0   | 53.2  |

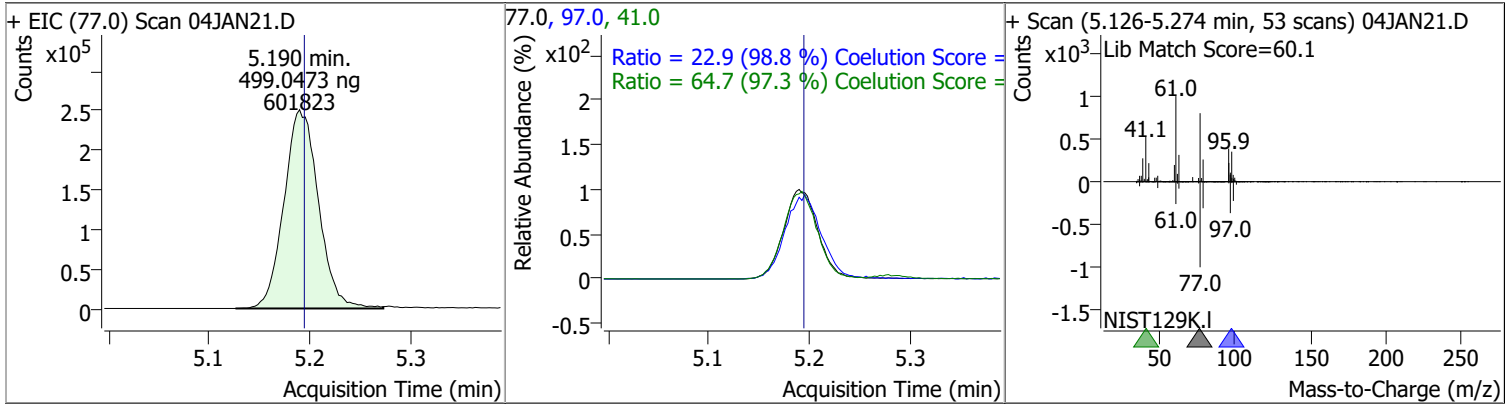


| Compound               | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,2-Dichloroethene | 516.0544 | 5.21 | 0.00     | 452377 | 61.0 | 166.1  | 137.2 | 197.2 |
|                        |          |      |          |        | 98.0 | 65.6   | 37.3  | 97.3  |

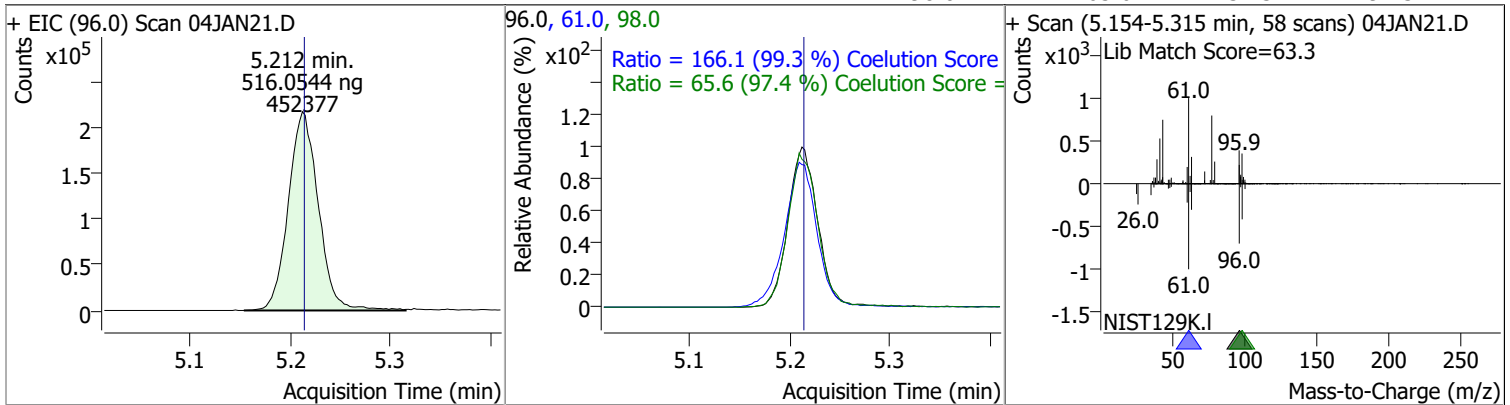

| Compound            | Conc.     | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|-----------|------|----------|--------|------|--------|-------|-------|
| Methyl ethyl ketone | 5327.1253 | 5.28 | 0.00     | 632539 | 72.0 | 21.6   | 0.0   | 51.3  |

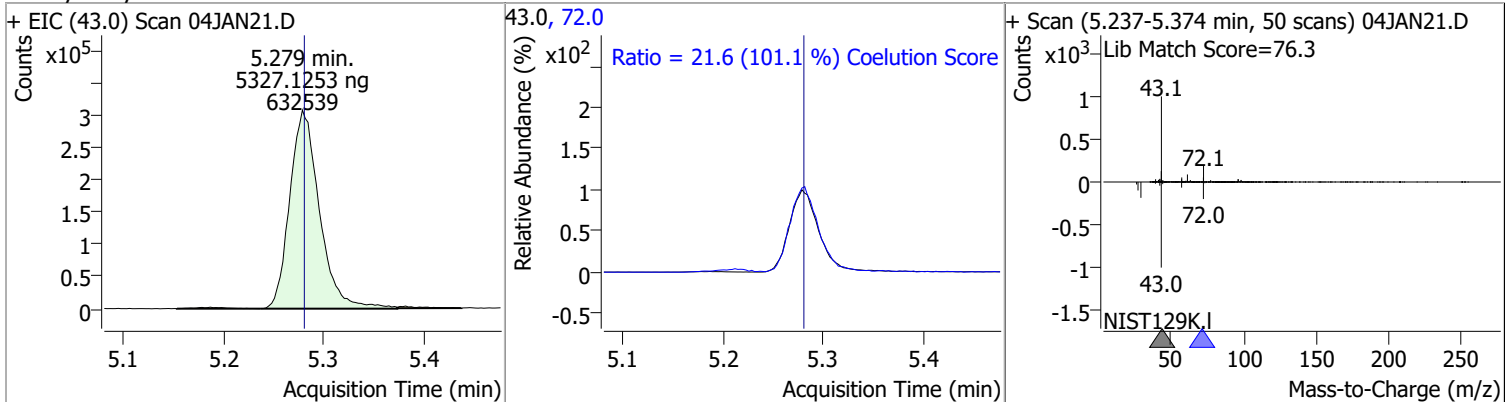


| Compound           | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| Bromochloromethane | 494.6054 | 5.52 | 0.00     | 179618 | 49.0 | 186.2  | 152.9 | 212.9 |

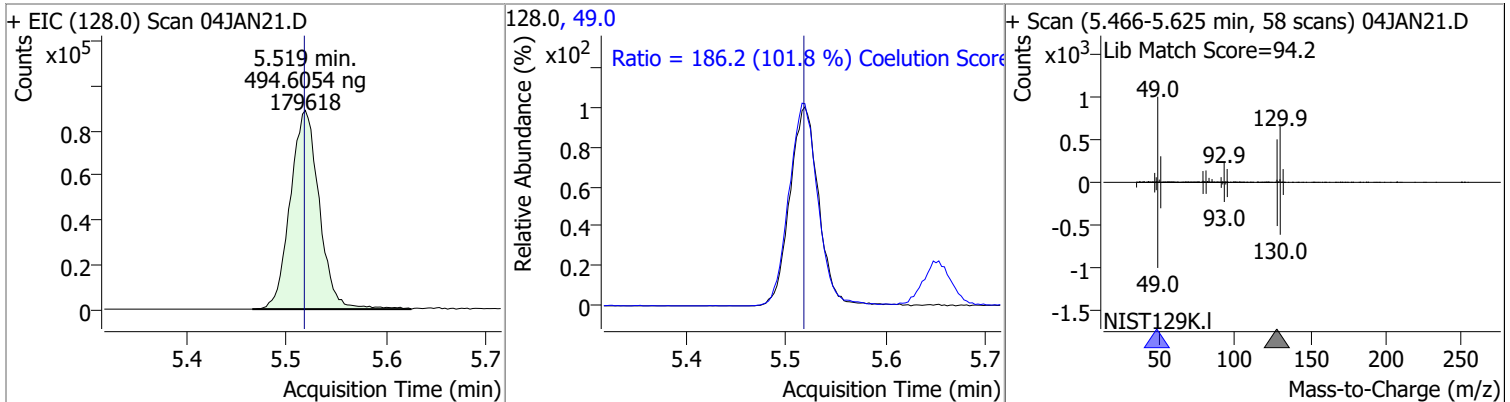


# Quantitation Results Report (QT Reviewed)


| Compound   | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|------|--------|-------|-------|
| Chloroform | 489.1221 | 5.65 | 0.00     | 783422 | 85.0 | 65.4   | 36.0  | 96.0  |




| Compound              | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1,1-Trichloroethane | 518.8312 | 5.83 | 0.00     | 778785 | 99.0 | 64.1   | 34.7  | 94.7  |
|                       |          |      |          |        | 61.0 | 48.2   | 18.1  | 78.1  |

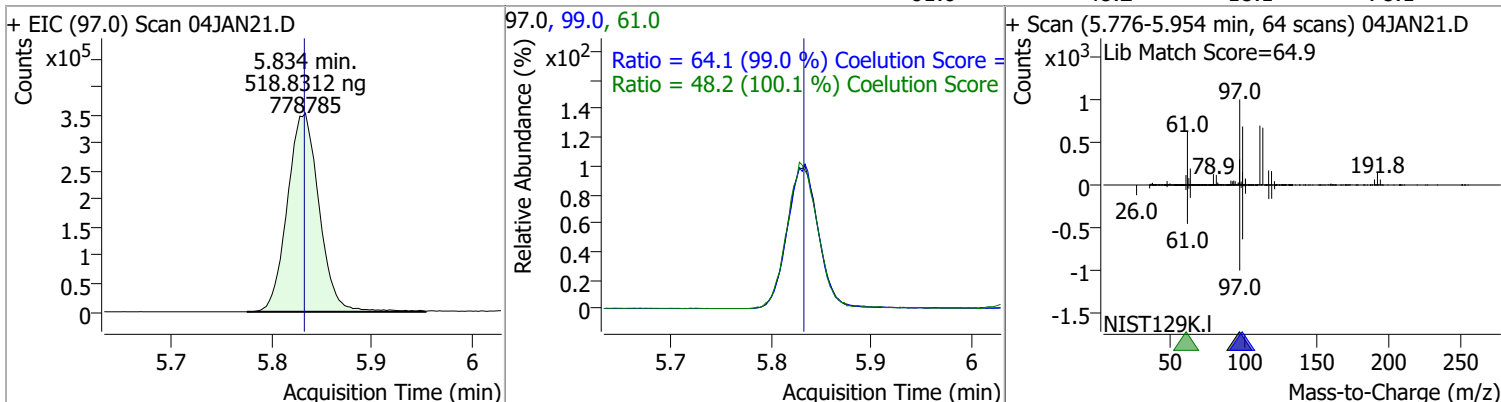

| Compound             | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Dibromofluoromethane | 510.3991 | 5.85 | 0.00     | 404568 | 191.5 | 22.4   | 0.0   | 53.1  |

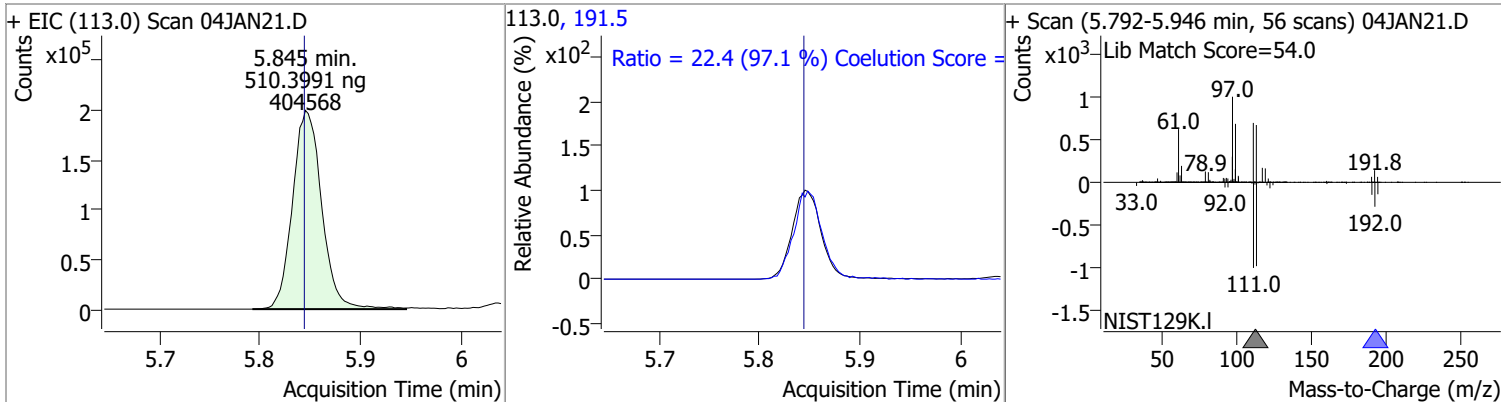


| Compound             | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Carbon tetrachloride | 521.2630 | 6.02 | 0.00     | 770907 | 119.0 | 95.3   | 67.2  | 127.2 |
|                      |          |      |          |        | 121.0 | 31.1   | 0.1   | 60.1  |

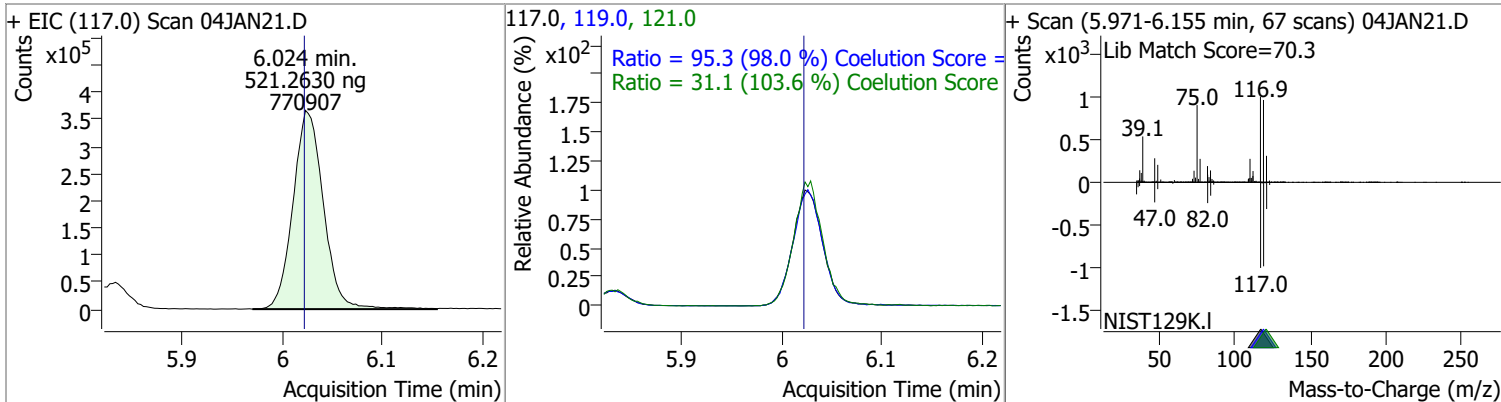


# Quantitation Results Report (QT Reviewed)


| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|-------|--------|-------|-------|
| 1,1-Dichloropropene | 543.5121 | 6.04 | 0.00     | 693669 | 110.0 | 35.6   | 5.9   | 65.9  |
|                     |          |      |          |        | 77.0  | 30.8   | 0.1   | 60.1  |

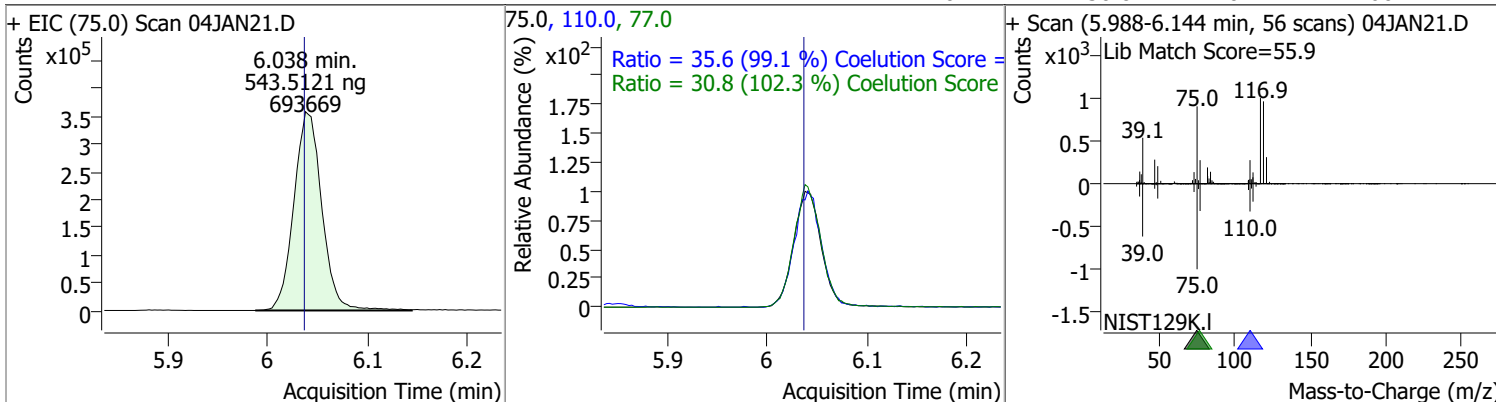


| Compound              | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 510.3080 | 6.23 | 0.00     | 174713 | 65.0 | 194.7  | 166.5 | 226.5 |

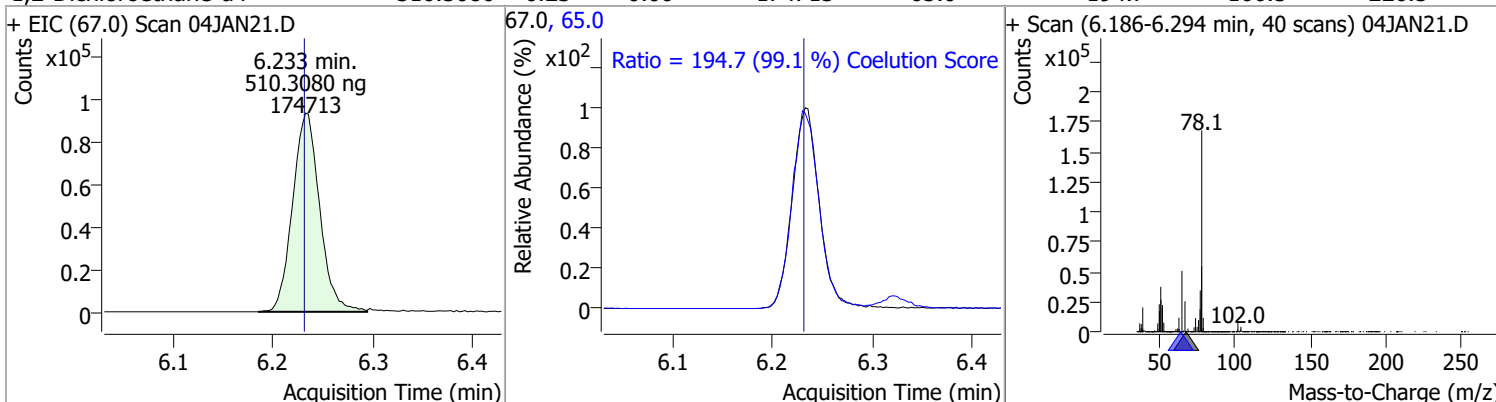

| Compound | Conc.    | RT   | Dev(Min) | Resp.   | QIon | QRatio | Lower | Upper |
|----------|----------|------|----------|---------|------|--------|-------|-------|
| Benzene  | 511.6658 | 6.28 | 0.00     | 1714050 | 77.0 | 23.5   | 0.0   | 53.5  |




| Compound           | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloroethane | 497.3699 | 6.32 | 0.00     | 450739 | 64.0 | 30.0   | 0.0   | 59.9  |
|                    |          |      |          |        | 98.0 | 7.4    | 0.0   | 37.6  |




# Quantitation Results Report (QT Reviewed)


| Compound        | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|-----------------|----------|------|----------|--------|-------|--------|-------|-------|
| Trichloroethene | 534.4007 | 7.03 | 0.00     | 505400 | 130.0 | 103.0  | 71.5  | 131.5 |
|                 |          |      |          |        | 97.0  | 65.2   | 34.1  | 94.1  |

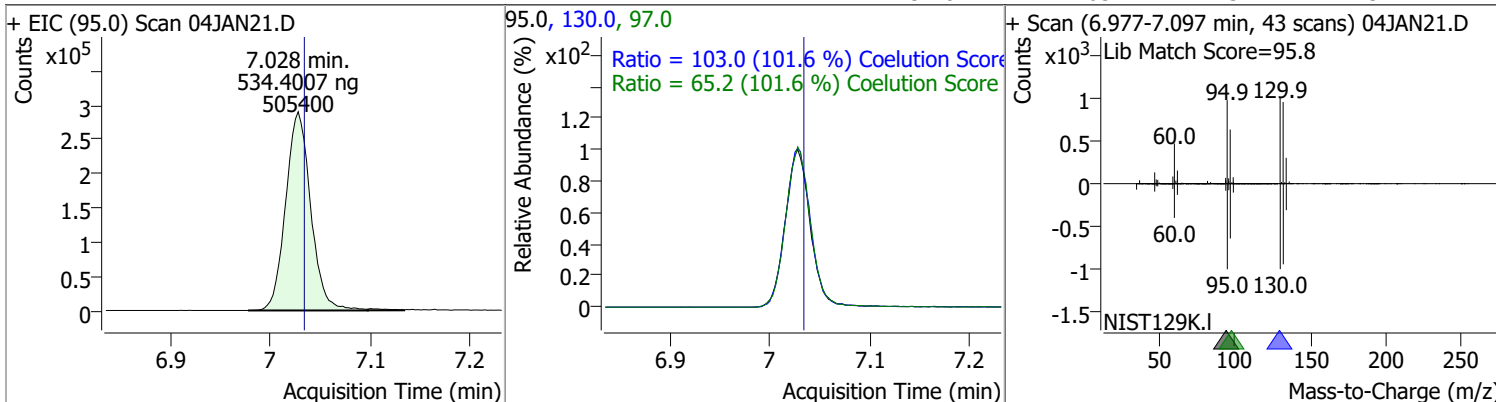

| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloropropane | 524.1695 | 7.27 | 0.00     | 436057 | 76.0 | 38.1   | 8.2   | 68.2  |

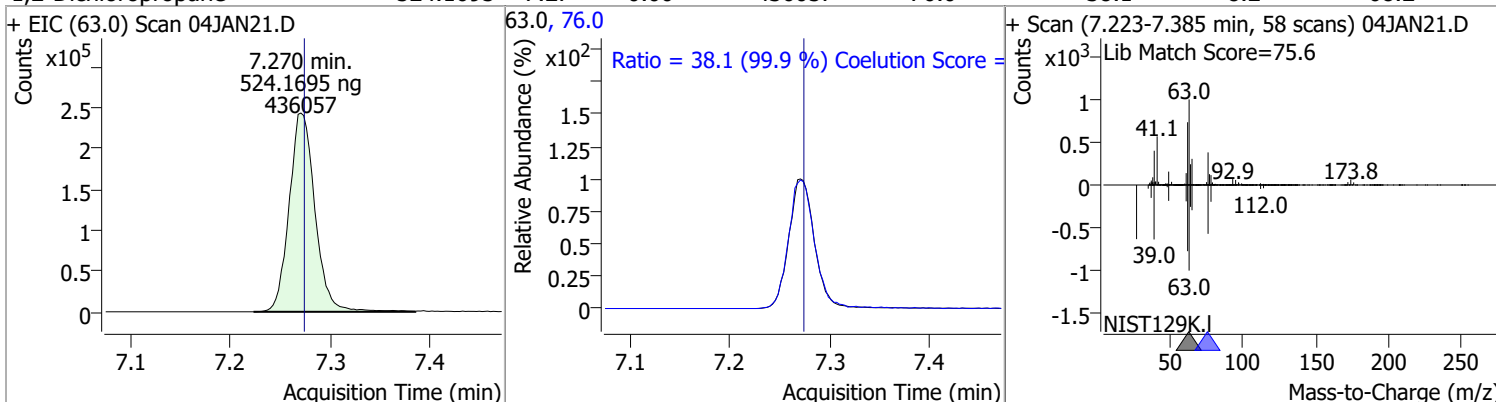




| Compound       | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------|----------|------|----------|--------|-------|--------|-------|-------|
| Dibromomethane | 500.7456 | 7.40 | 0.00     | 176038 | 173.5 | 109.8  | 83.7  | 143.7 |
|                |          |      |          |        | 95.0  | 82.8   | 52.2  | 112.2 |

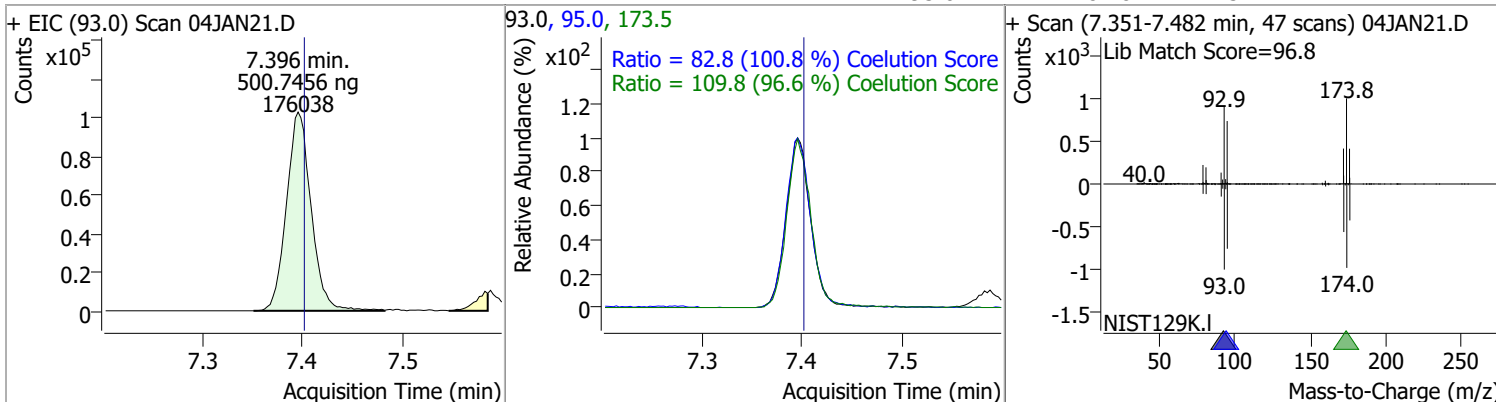






# Quantitation Results Report (QT Reviewed)




| Compound             | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Bromodichloromethane | 518.3718 | 7.59 | 0.00     | 502929 | 85.0  | 64.7   | 34.5  | 94.5  |
|                      |          |      |          |        | 127.0 | 9.4    | 0.0   | 39.6  |



| Compound                | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|-------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,3-Dichloropropene | 538.9008 | 8.06 | 0.00     | 591147 | 39.0 | 52.4   | 23.3  | 83.3  |
|                         |          |      |          |        | 77.0 | 31.4   | 1.0   | 61.0  |



| Compound   | Conc.    | RT   | Dev(Min) | Resp.   | QIon  | QRatio | Lower | Upper |
|------------|----------|------|----------|---------|-------|--------|-------|-------|
| Toluene-d8 | 544.2136 | 8.32 | 0.00     | 1644540 | 100.0 | 64.1   | 34.4  | 94.4  |
|            |          |      |          |         | 99.0  | 9.5    | 0.0   | 39.6  |




# Quantitation Results Report (QT Reviewed)


| Compound                    | Conc.    | RT   | Dev(Min)         | Resp.   | QIon | QRatio                                       | Lower | Upper |
|-----------------------------|----------|------|------------------|---------|------|----------------------------------------------|-------|-------|
| Toluene                     | 536.5101 | 8.39 | 0.00             | 1095161 | 91.0 | 174.1                                        | 145.8 | 205.8 |
| + EIC (92.0) Scan 04JAN21.D |          |      | 92.0, 91.0       |         |      | + Scan (8.341-8.542 min, 73 scans) 04JAN21.D |       |       |
|                             |          |      |                  |         |      |                                              |       |       |
| trans-1,3-Dichloropropene   | 533.7551 | 8.64 | 0.00             | 416771  | 39.0 | 52.3                                         | 23.4  | 83.4  |
|                             |          |      |                  |         | 77.0 | 33.0                                         | 2.4   | 62.4  |
| + EIC (75.0) Scan 04JAN21.D |          |      | 75.0, 77.0, 39.0 |         |      | + Scan (8.598-8.715 min, 43 scans) 04JAN21.D |       |       |
|                             |          |      |                  |         |      |                                              |       |       |
| 1,1,2-Trichloroethane       | 505.1803 | 8.82 | 0.00             | 205463  | 97.0 | 112.6                                        | 84.6  | 144.6 |
|                             |          |      |                  |         | 85.0 | 63.1                                         | 37.6  | 97.6  |
| + EIC (83.0) Scan 04JAN21.D |          |      | 83.0, 97.0, 85.0 |         |      | + Scan (8.768-8.907 min, 51 scans) 04JAN21.D |       |       |
|                             |          |      |                  |         |      |                                              |       |       |

# Quantitation Results Report (QT Reviewed)


| Compound          | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|-------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Tetrachloroethene | 514.9255 | 8.94 | 0.00     | 428812 | 165.8 | 129.5  | 98.6  | 158.6 |
|                   |          |      |          |        | 129.0 | 91.5   | 61.5  | 121.5 |




| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,3-Dichloropropane | 511.2479 | 8.98 | 0.00     | 408993 | 78.0 | 32.9   | 2.9   | 62.9  |







| Compound             | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Chlorodibromomethane | 520.4361 | 9.20 | 0.00     | 330813 | 127.0 | 76.7   | 48.0  | 108.0 |



| Compound          | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|-------------------|----------|------|----------|--------|-------|--------|-------|-------|
| 1,2-Dibromoethane | 507.9234 | 9.30 | 0.00     | 225877 | 109.0 | 95.9   | 64.5  | 124.5 |




# Quantitation Results Report (QT Reviewed)

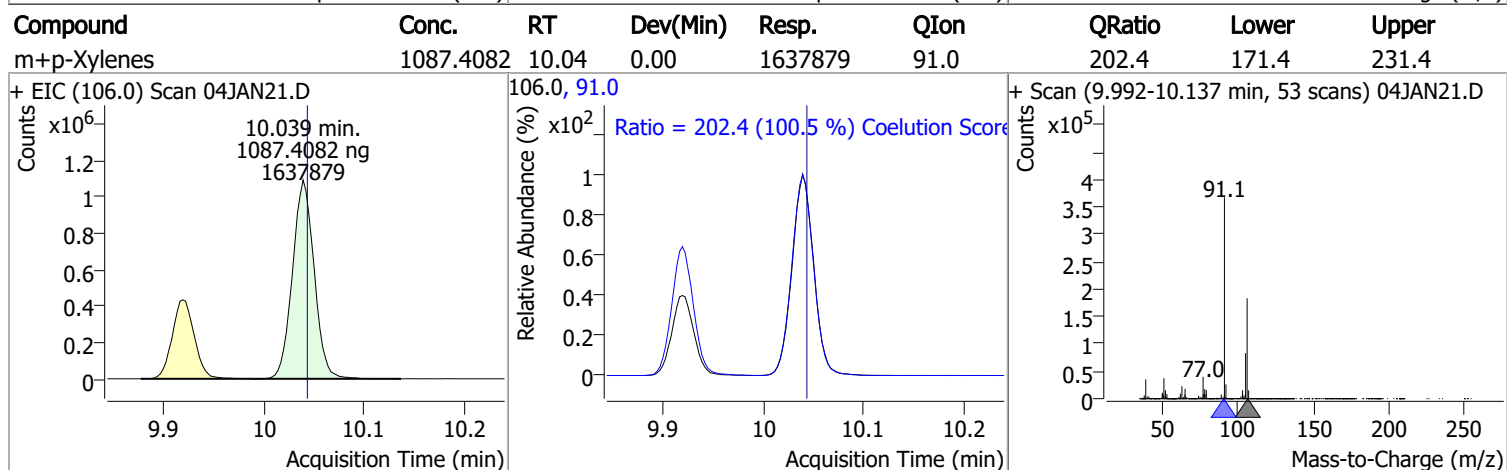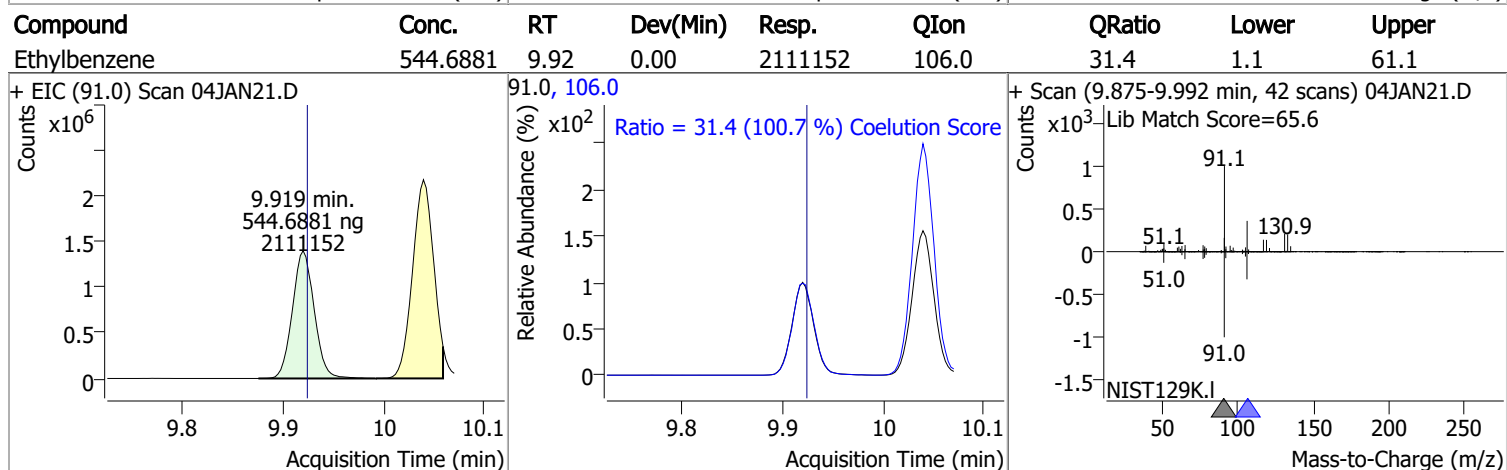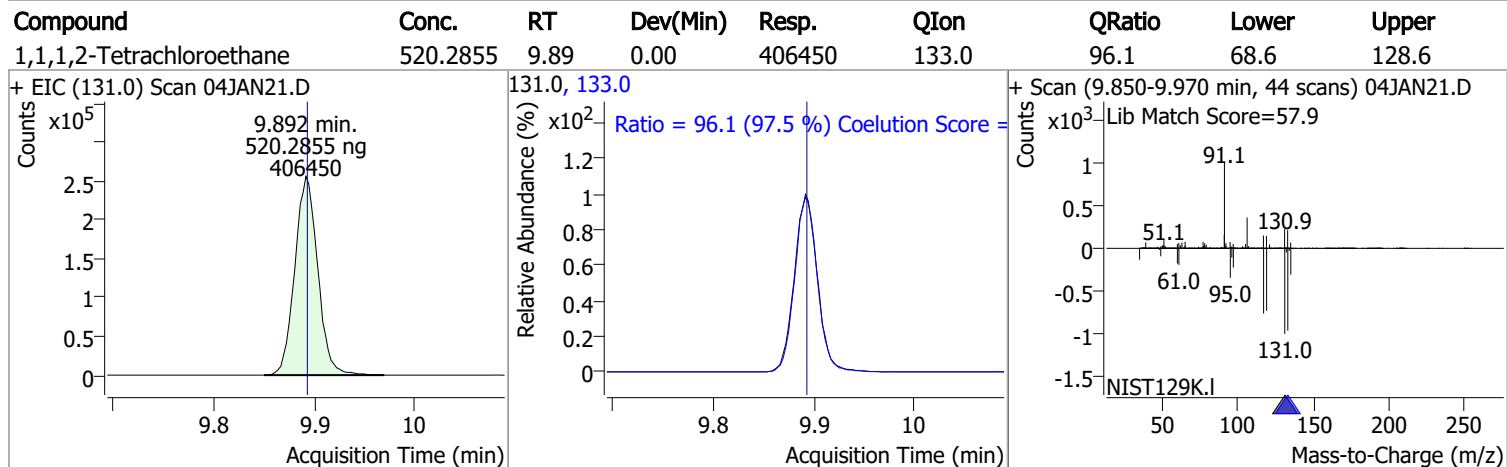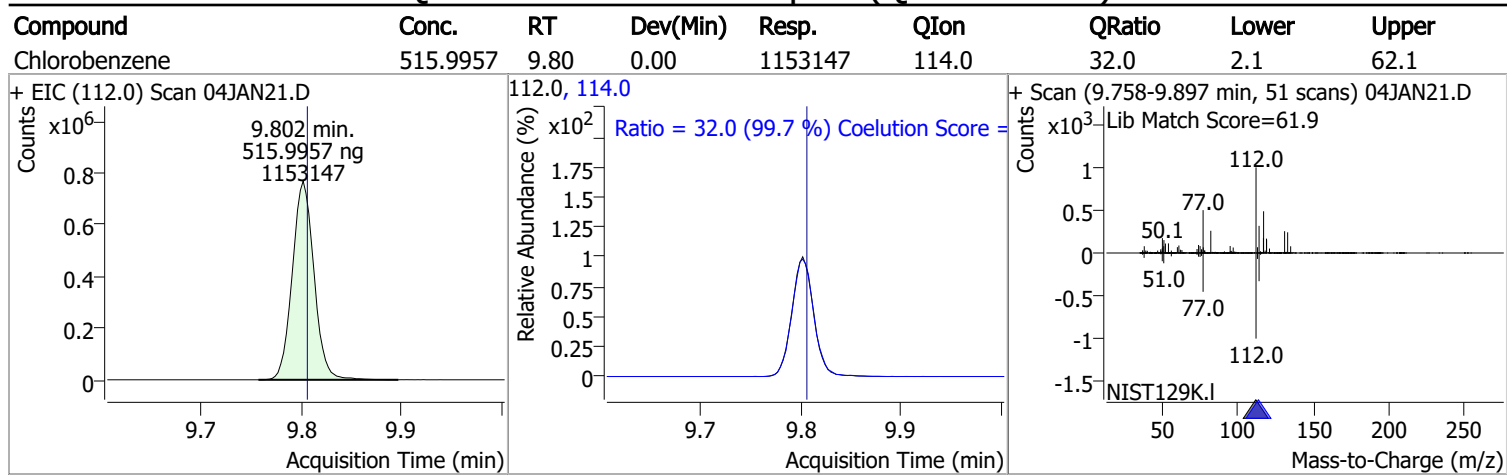


# Quantitation Results Report (QT Reviewed)


| Compound | Conc.    | RT    | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|----------|----------|-------|----------|--------|------|--------|-------|-------|
| o-Xylene | 547.4764 | 10.43 | 0.00     | 734101 | 91.0 | 213.0  | 183.1 | 243.1 |

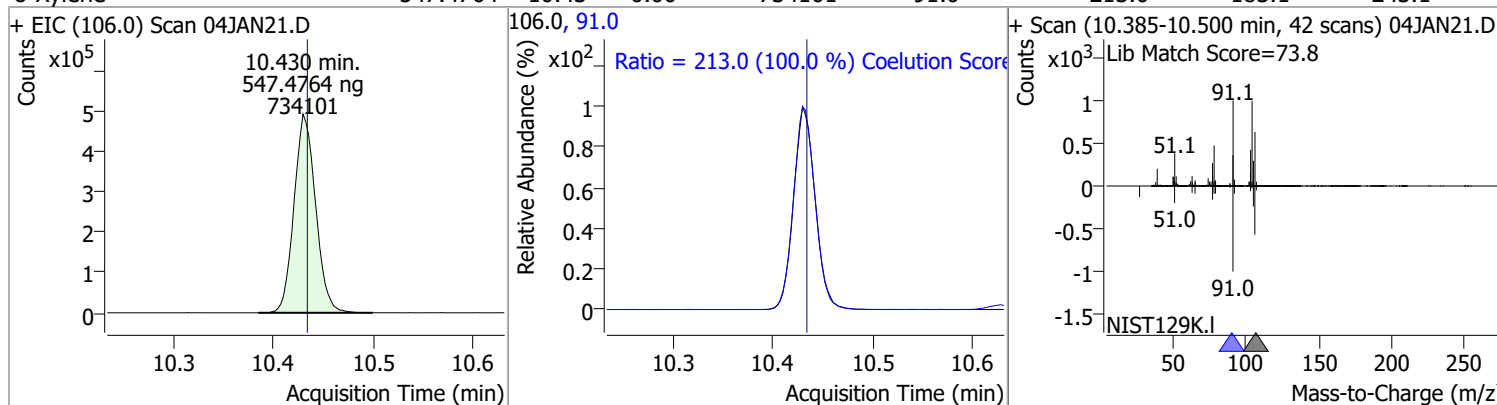


| Compound | Conc.    | RT    | Dev(Min) | Resp.   | QIon | QRatio | Lower | Upper |
|----------|----------|-------|----------|---------|------|--------|-------|-------|
| Styrene  | 555.7946 | 10.45 | 0.00     | 1199879 | 78.0 | 50.2   | 19.6  | 79.6  |

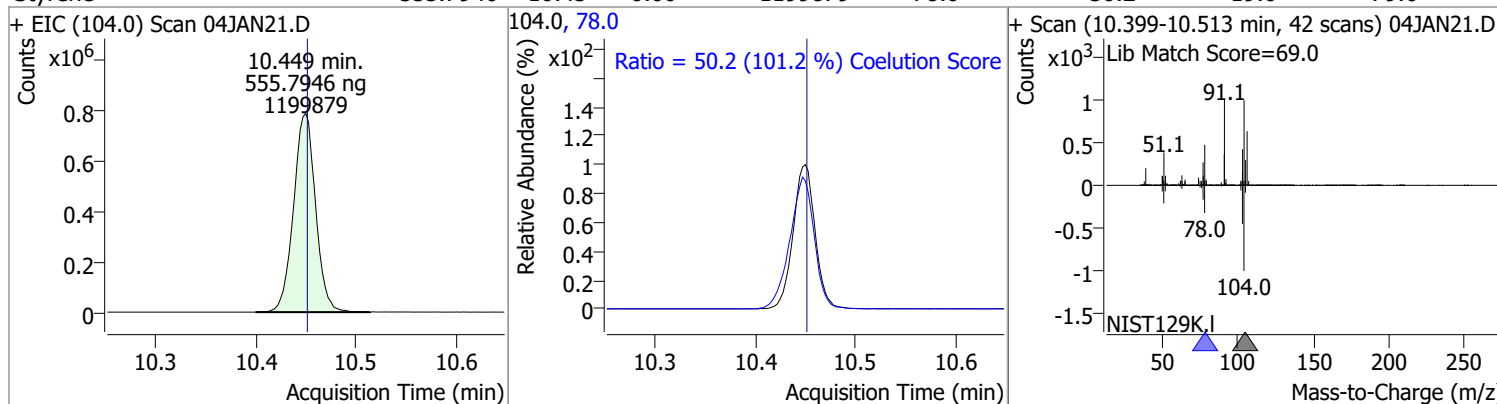

| Compound  | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|-----------|----------|-------|----------|--------|-------|--------|-------|-------|
| Bromoform | 522.7660 | 10.63 | 0.00     | 175918 | 170.5 | 51.3   | 22.1  | 82.1  |
|           |          |       |          |        | 174.5 | 48.1   | 20.1  | 80.1  |

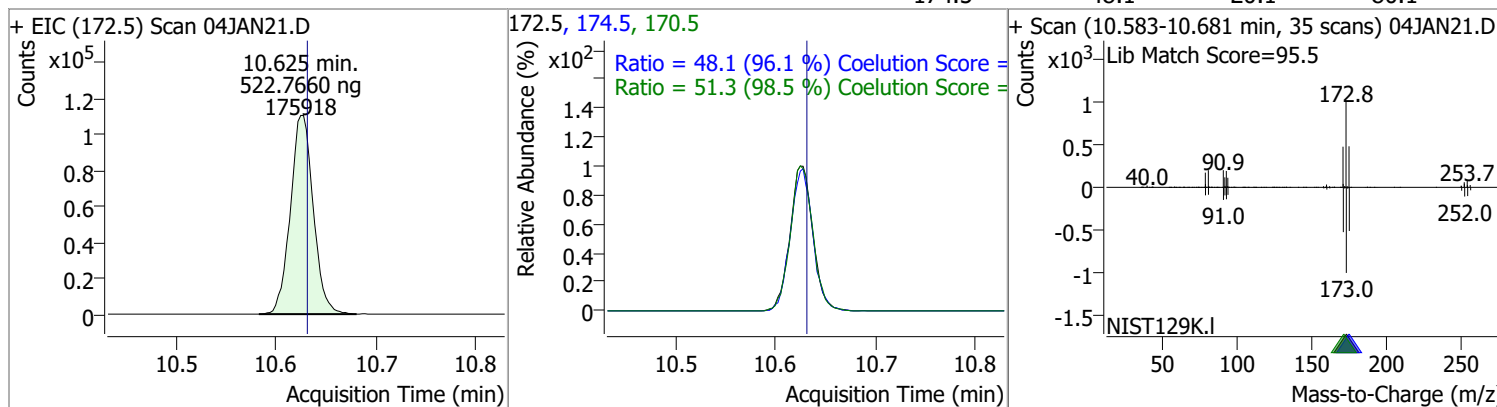


| Compound             | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 541.3964 | 10.95 | -0.01    | 521580 | 174.0 | 93.3   | 61.7  | 121.7 |
|                      |          |       |          |        | 176.0 | 89.7   | 60.6  | 120.6 |




# Quantitation Results Report (QT Reviewed)


| Compound     | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|--------------|----------|-------|----------|--------|-------|--------|-------|-------|
| Bromobenzene | 516.0104 | 11.09 | 0.00     | 439147 | 77.0  | 142.6  | 115.7 | 175.7 |
|              |          |       |          |        | 158.0 | 97.9   | 66.5  | 126.5 |

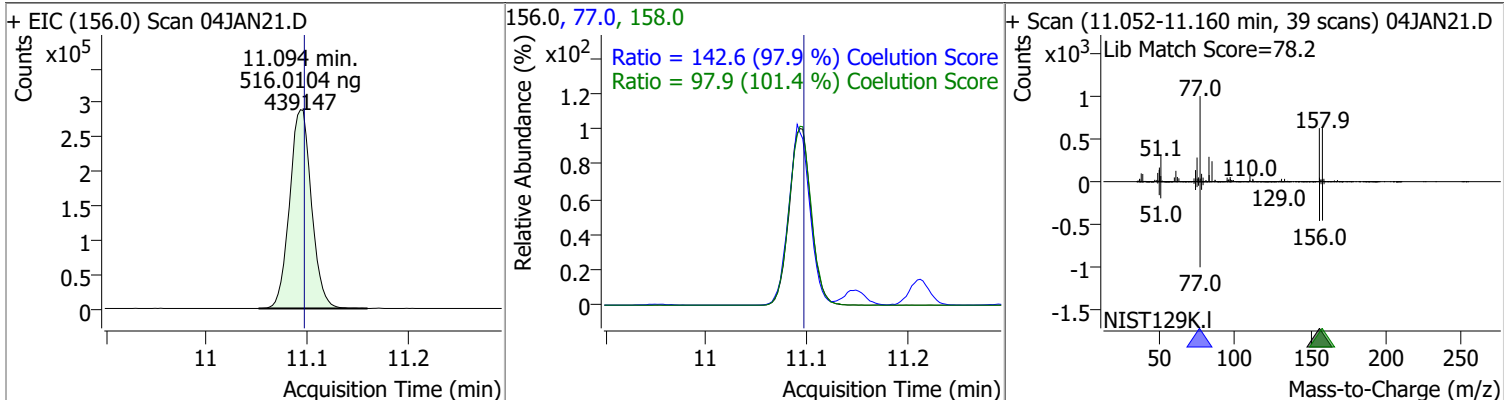


| Compound                  | Conc.    | RT    | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------------|----------|-------|----------|--------|------|--------|-------|-------|
| 1,1,2,2-Tetrachloroethane | 491.6700 | 11.11 | 0.00     | 240837 | 85.0 | 65.5   | 36.2  | 96.2  |

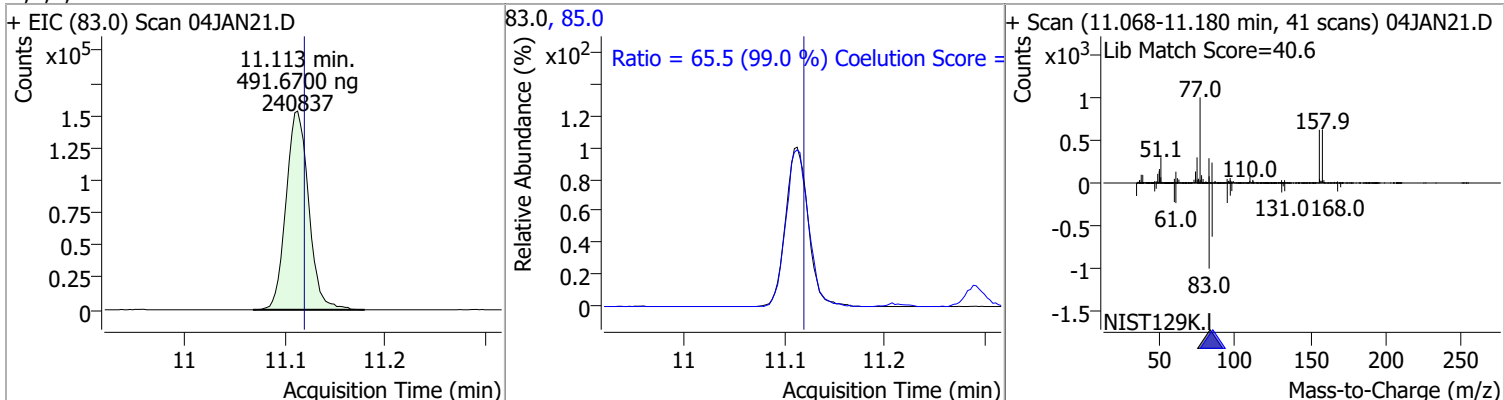

| Compound               | Conc.    | RT    | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|------------------------|----------|-------|----------|-------|-------|--------|-------|-------|
| 1,2,3-Trichloropropane | 491.5229 | 11.15 | 0.00     | 64422 | 112.0 | 62.7   | 33.5  | 93.5  |






| Compound        | Conc.    | RT    | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|-----------------|----------|-------|----------|--------|------|--------|-------|-------|
| 2-Chlorotoluene | 538.4964 | 11.29 | 0.00     | 455991 | 91.0 | 280.4  | 252.3 | 312.3 |






# Quantitation Results Report (QT Reviewed)




| Compound        | Conc.    | RT    | Dev(Min) | Resp.   | QIon  | QRatio | Lower | Upper |
|-----------------|----------|-------|----------|---------|-------|--------|-------|-------|
| 4-Chlorotoluene | 531.8471 | 11.40 | 0.00     | 1468376 | 126.0 | 31.7   | 1.7   | 61.7  |



| Compound            | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,3-Dichlorobenzene | 511.5504 | 12.03 | 0.00     | 793993 | 148.0 | 63.7   | 33.6  | 93.6  |
|                     |          |       |          |        | 111.0 | 39.5   | 9.8   | 69.8  |






| Compound            | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,4-Dichlorobenzene | 502.3001 | 12.13 | 0.00     | 794954 | 148.0 | 63.9   | 33.1  | 93.1  |
|                     |          |       |          |        | 111.0 | 38.5   | 9.1   | 69.1  |



# Quantitation Results Report (QT Reviewed)


| Compound            | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,2-Dichlorobenzene | 506.3871 | 12.49 | 0.00     | 664247 | 148.0 | 64.3   | 33.9  | 93.9  |
|                     |          |       |          |        | 111.0 | 40.6   | 11.0  | 71.0  |

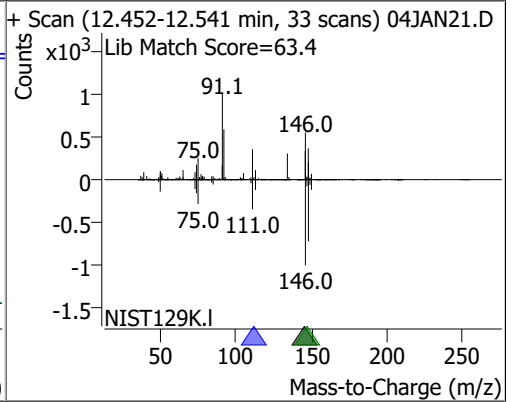



# Quantitation Results Report (QT Reviewed)

|                |                                     |                   |                       |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File      | 04JAN23.D                           | Operator          | MSC                   |
| Acq. Method    | 5975CACQF.M                         | Acq. Date-Time    | 1/4/2022 9:29:14 PM   |
| Sample Name    | ICV010422                           | Instrument        | VOA5975C              |
| Vial           | 23                                  | Multiplier        | 1.00                  |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m  | Comment           |                       |
| Tune File      | BFB_Atune3.u                        | Tune Date         | 10/11/2021 4:02:00 PM |
| Batch Name     | VG010422_8260B.batch.bin            | Last Calib Update | 1/9/2022 8:59:52 PM   |
| Ref Library    | \\MASSHUNTER\Org\Library\NIST129K.I |                   |                       |

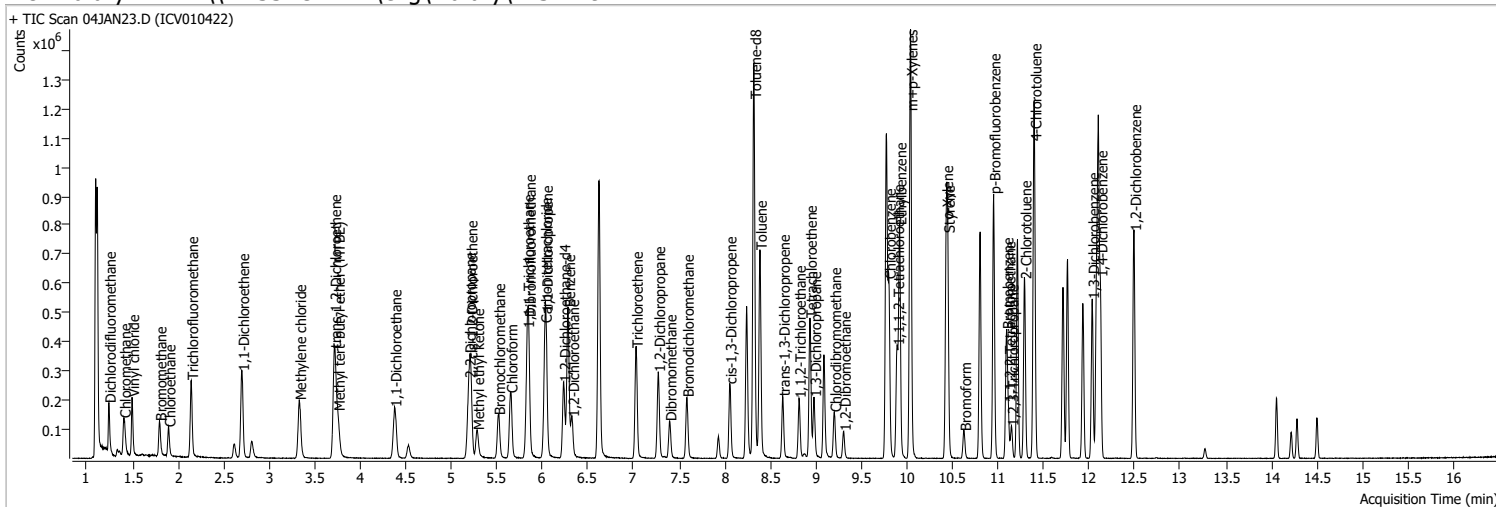

| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|----------|----|------|-------|-------|-------|----------|
|----------|----|------|-------|-------|-------|----------|

**Internal Standards**

|                          |        |       |        |          |    |        |
|--------------------------|--------|-------|--------|----------|----|--------|
| M Fluorobenzene          | 6.621  | 96.0  | 801210 | 250.0000 | ng | -0.003 |
| M Chlorobenzene-d5       | 9.774  | 82.0  | 307868 | 250.0000 | ng | 0.003  |
| M 1,4-Dichlorobenzene-d4 | 12.100 | 152.0 | 255907 | 250.0000 | ng | 0.000  |

**System Monitoring Compounds**

|                         |                      |       |        |                    |    |        |
|-------------------------|----------------------|-------|--------|--------------------|----|--------|
| S Dibromofluoromethane  | 5.848                | 113.0 | 204707 | 271.1994           | ng | 0.003  |
| Spiked Amount: 250.000  | Range: 80.0 - 119.0% |       |        | Recovery = 108.48% |    |        |
| S 1,2-Dichloroethane-d4 | 6.230                | 67.0  | 91382  | 280.2886           | ng | -0.003 |
| Spiked Amount: 250.000  | Range: 81.0 - 118.0% |       |        | Recovery = 112.12% |    |        |
| S Toluene-d8            | 8.322                | 98.0  | 821531 | 276.9106           | ng | 0.003  |
| Spiked Amount: 250.000  | Range: 89.0 - 112.0% |       |        | Recovery = 110.76% |    |        |
| S p-Bromofluorobenzene  | 10.951               | 95.0  | 253034 | 269.8976           | ng | -0.003 |
| Spiked Amount: 250.000  | Range: 85.0 - 114.0% |       |        | Recovery = 107.96% |    |        |

**Target Compounds**









| Compound                         | RT    | QIon  | Resp.  | Conc.     | Units | QValue |
|----------------------------------|-------|-------|--------|-----------|-------|--------|
| T Dichlorodifluoromethane        | 1.241 | 85.0  | 116936 | 111.3749  | ng    | 99     |
| T Chloromethane                  | 1.406 | 50.0  | 138617 | 108.7739  | ng    | 98     |
| T Vinyl chloride                 | 1.495 | 62.0  | 137775 | 120.1518  | ng    | 86     |
| T Bromomethane                   | 1.796 | 96.0  | 59947  | 116.9157  | ng    | 100    |
| T Chloroethane                   | 1.897 | 64.0  | 65619  | 115.5932  | ng    | 99     |
| T Trichlorofluoromethane         | 2.145 | 101.0 | 173333 | 121.7847  | ng    | 97     |
| T 1,1-Dichloroethene             | 2.702 | 96.0  | 108512 | 134.4566  | ng    | 100    |
| T Methylene chloride             | 3.330 | 49.0  | 144585 | 121.5297  | ng    | 98     |
| T trans-1,2-Dichloroethene       | 3.715 | 96.0  | 110909 | 134.7028  | ng    | 98     |
| T Methyl tert-butyl ether (MTBE) | 3.754 | 73.0  | 143378 | 134.7224  | ng    | 99     |
| T 1,1-Dichloroethane             | 4.376 | 63.0  | 208131 | 135.8030  | ng    | 98     |
| T 2,2-Dichloropropane            | 5.190 | 77.0  | 150902 | 131.4031  | ng    | 97     |
| T cis-1,2-Dichloroethene         | 5.209 | 96.0  | 108623 | 130.1231  | ng    | 99     |
| T Methyl ethyl ketone            | 5.282 | 43.0  | 135511 | 1198.4439 | ng    | 98     |
| T Bromochloromethane             | 5.513 | 128.0 | 42744  | 123.6009  | ng    | 99     |
| T Chloroform                     | 5.647 | 83.0  | 183676 | 120.4236  | ng    | 100    |

# Quantitation Results Report (QT Reviewed)





| Compound                    | RT     | QIon  | Resp.  | Conc.    | Units | Dev(Min) |
|-----------------------------|--------|-------|--------|----------|-------|----------|
| T 1,1,1-Trichloroethane     | 5.831  | 97.0  | 183324 | 128.2524 | ng    | 99       |
| T Carbon tetrachloride      | 6.027  | 117.0 | 181384 | 128.7928 | ng    | 99       |
| T 1,1-Dichloropropene       | 6.038  | 75.0  | 150930 | 124.1853 | ng    | 100      |
| T Benzene                   | 6.280  | 78.0  | 418900 | 131.3139 | ng    | 99       |
| T 1,2-Dichloroethane        | 6.325  | 62.0  | 104249 | 120.7991 | ng    | 95       |
| T Trichloroethene           | 7.025  | 95.0  | 121734 | 131.1096 | ng    | 99       |
| T 1,2-Dichloropropane       | 7.270  | 63.0  | 102633 | 125.6626 | ng    | 99       |
| T Dibromomethane            | 7.393  | 93.0  | 43248  | 125.3047 | ng    | 97       |
| T Bromodichloromethane      | 7.585  | 83.0  | 122757 | 128.8759 | ng    | 100      |
| T cis-1,3-Dichloropropene   | 8.054  | 75.0  | 130910 | 121.5561 | ng    | 98       |
| T Toluene                   | 8.386  | 92.0  | 264584 | 132.0244 | ng    | 100      |
| T trans-1,3-Dichloropropene | 8.637  | 75.0  | 98907  | 129.0216 | ng    | 97       |
| T 1,1,2-Trichloroethane     | 8.815  | 83.0  | 49128  | 123.0361 | ng    | 98       |
| T Tetrachloroethene         | 8.935  | 163.8 | 103027 | 126.0141 | ng    | 99       |
| T 1,3-Dichloropropane       | 8.980  | 76.0  | 95697  | 121.8442 | ng    | 98       |
| T Chlorodibromomethane      | 9.203  | 129.0 | 78076  | 125.1103 | ng    | 98       |
| T 1,2-Dibromoethane         | 9.306  | 107.0 | 54259  | 124.2764 | ng    | 100      |
| T Chlorobenzene             | 9.802  | 112.0 | 288815 | 131.6352 | ng    | 99       |
| T 1,1,1,2-Tetrachloroethane | 9.892  | 131.0 | 97148  | 126.6657 | ng    | 95       |
| T Ethylbenzene              | 9.917  | 91.0  | 501953 | 131.9113 | ng    | 99       |
| T m+p-Xylenes               | 10.039 | 106.0 | 388558 | 262.7589 | ng    | 100      |
| T o-Xylene                  | 10.430 | 106.0 | 174061 | 132.2214 | ng    | 98       |
| T Styrene                   | 10.449 | 104.0 | 291425 | 137.4974 | ng    | 98       |
| T Bromoform                 | 10.628 | 172.5 | 42560  | 129.9644 | ng    | 98       |
| T Bromobenzene              | 11.093 | 156.0 | 109054 | 131.6788 | ng    | 99       |
| T 1,1,2,2-Tetrachloroethane | 11.113 | 83.0  | 60763  | 127.4722 | ng    | 98       |
| T 1,2,3-Trichloropropane    | 11.146 | 110.0 | 15682  | 122.9523 | ng    | 99       |
| T 2-Chlorotoluene           | 11.291 | 126.0 | 108192 | 131.2948 | ng    | 95       |
| T 4-Chlorotoluene           | 11.400 | 91.0  | 368295 | 137.0790 | ng    | 100      |
| T 1,3-Dichlorobenzene       | 12.033 | 146.0 | 204088 | 135.1185 | ng    | 99       |
| T 1,4-Dichlorobenzene       | 12.122 | 146.0 | 200032 | 129.8812 | ng    | 99       |
| T 1,2-Dichlorobenzene       | 12.493 | 146.0 | 164299 | 128.7104 | ng    | 99       |

(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (\*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

# Quantitation Results Report (QT Reviewed)

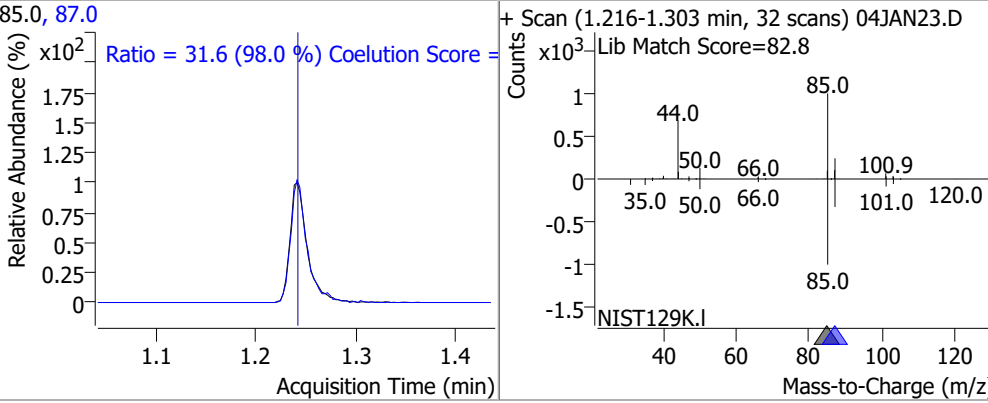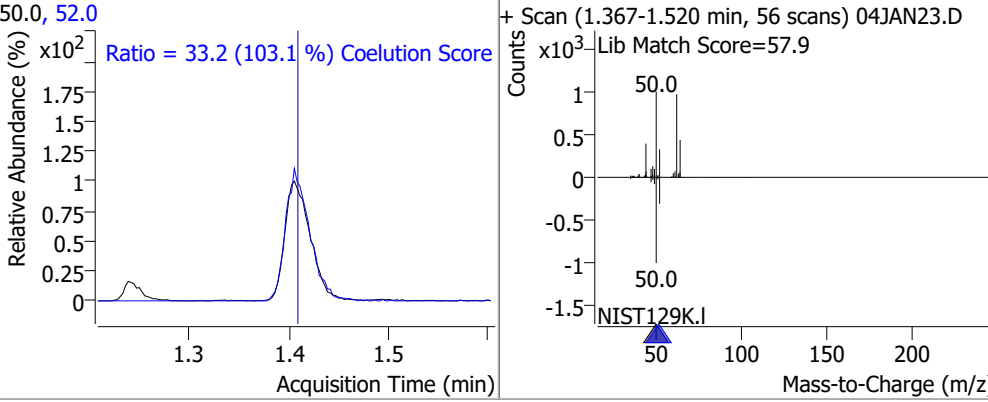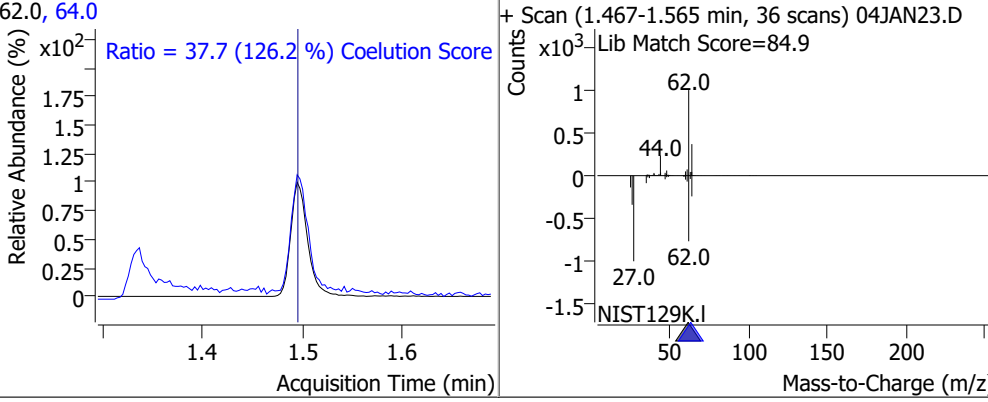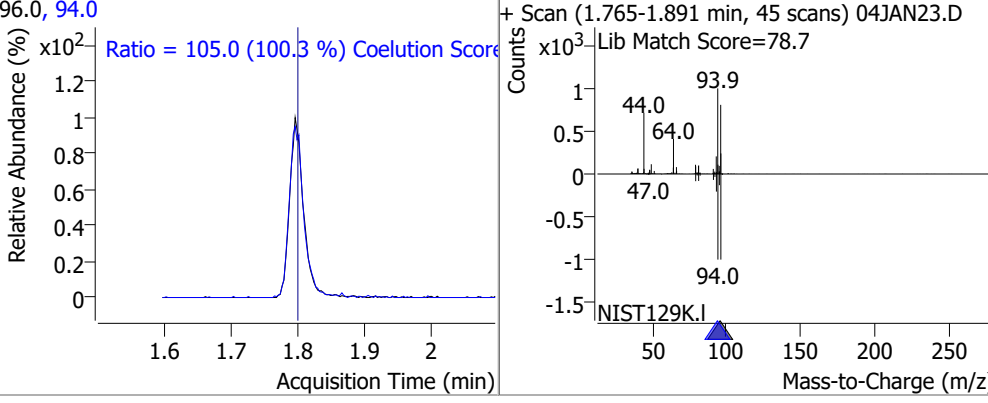
| Compound                                                                           | Conc.                                     | RT   | Dev(Min)                                                                             | Resp.  | QIon | QRatio                                       | Lower | Upper |
|------------------------------------------------------------------------------------|-------------------------------------------|------|--------------------------------------------------------------------------------------|--------|------|----------------------------------------------|-------|-------|
| Dichlorodifluoromethane                                                            | 111.3749                                  | 1.24 | 0.00                                                                                 | 116936 | 87.0 | 31.6                                         | 2.3   | 62.3  |
| + EIC (85.0) Scan 04JAN23.D                                                        |                                           |      | 85.0, 87.0                                                                           |        |      | + Scan (1.216-1.303 min, 32 scans) 04JAN23.D |       |       |
|    | Ratio = 31.6 (98.0 %) Coelution Score =   |      |    |        |      |                                              |       |       |
| Chloromethane                                                                      | 108.7739                                  | 1.41 | 0.00                                                                                 | 138617 | 52.0 | 33.2                                         | 2.1   | 62.1  |
| + EIC (50.0) Scan 04JAN23.D                                                        |                                           |      | 50.0, 52.0                                                                           |        |      | + Scan (1.367-1.520 min, 56 scans) 04JAN23.D |       |       |
|   | Ratio = 33.2 (103.1 %) Coelution Score =  |      |   |        |      |                                              |       |       |
| Vinyl chloride                                                                     | 120.1518                                  | 1.49 | 0.00                                                                                 | 137775 | 64.0 | 37.7                                         | 0.0   | 59.9  |
| + EIC (62.0) Scan 04JAN23.D                                                        |                                           |      | 62.0, 64.0                                                                           |        |      | + Scan (1.467-1.565 min, 36 scans) 04JAN23.D |       |       |
|  | Ratio = 37.7 (126.2 %) Coelution Score =  |      |  |        |      |                                              |       |       |
| Bromomethane                                                                       | 116.9157                                  | 1.80 | 0.00                                                                                 | 59947  | 94.0 | 105.0                                        | 74.6  | 134.6 |
| + EIC (96.0) Scan 04JAN23.D                                                        |                                           |      | 96.0, 94.0                                                                           |        |      | + Scan (1.765-1.891 min, 45 scans) 04JAN23.D |       |       |
|  | Ratio = 105.0 (100.3 %) Coelution Score = |      |  |        |      |                                              |       |       |

# Quantitation Results Report (QT Reviewed)

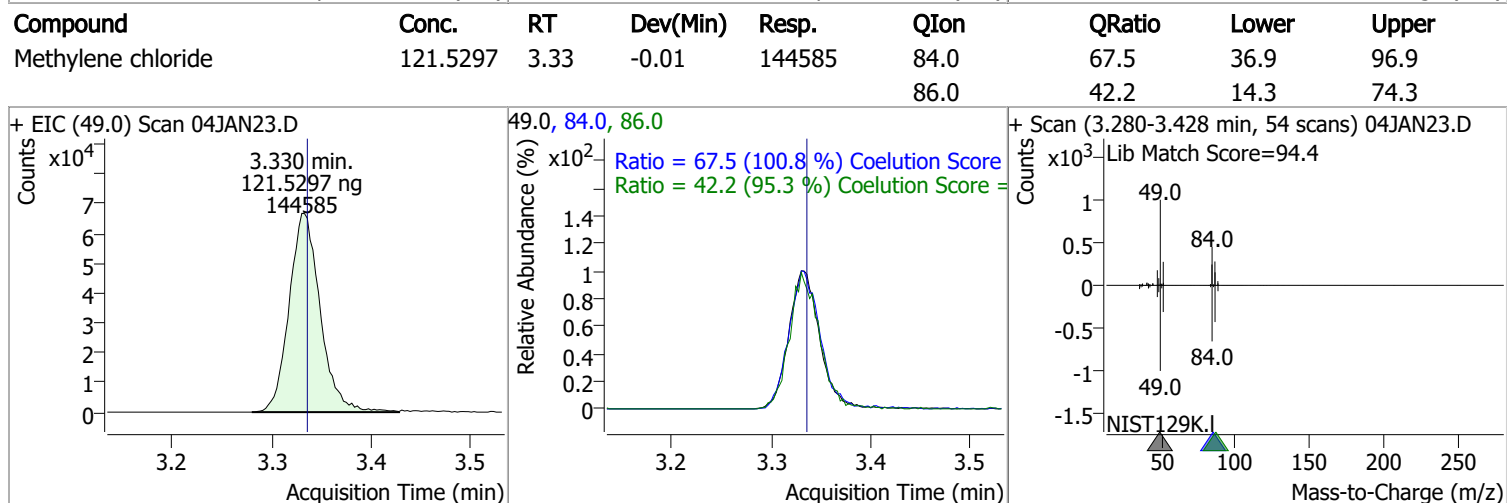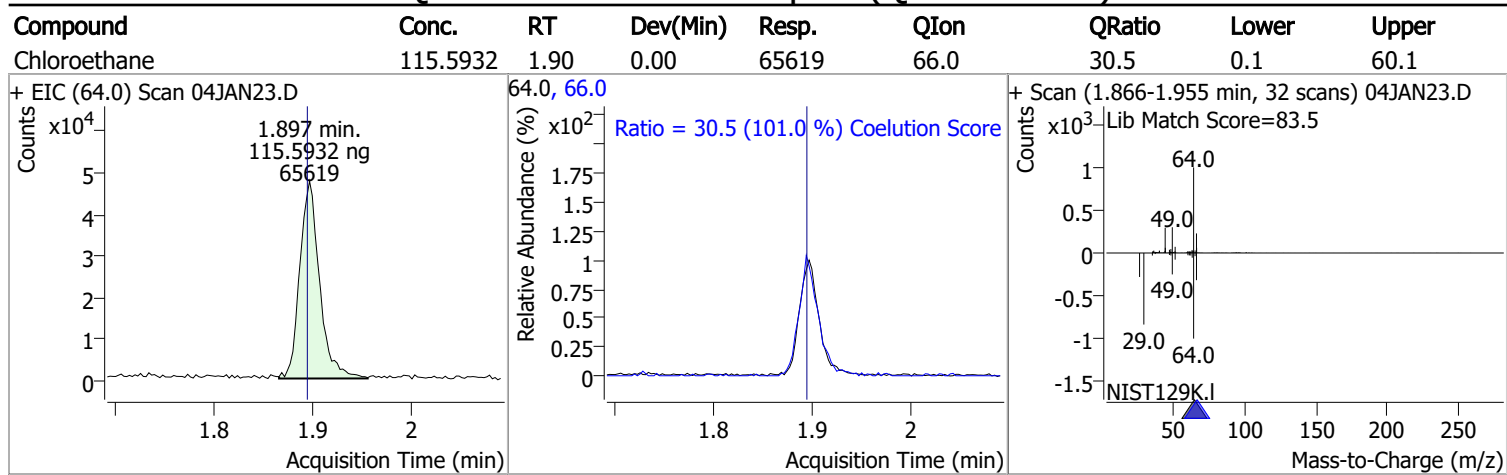


# Quantitation Results Report (QT Reviewed)


| Compound                 | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------------|----------|------|----------|--------|------|--------|-------|-------|
| trans-1,2-Dichloroethene | 134.7028 | 3.71 | 0.00     | 110909 | 61.0 | 156.1  | 123.9 | 183.9 |
|                          |          |      |          |        | 98.0 | 64.1   | 35.7  | 95.7  |



| Compound                       | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------------------|----------|------|----------|--------|------|--------|-------|-------|
| Methyl tert-butyl ether (MTBE) | 134.7224 | 3.75 | 0.00     | 143378 | 57.0 | 25.1   | 0.0   | 54.6  |




| Compound           | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1-Dichloroethane | 135.8030 | 4.38 | 0.00     | 208131 | 65.0 | 31.2   | 2.1   | 62.1  |
|                    |          |      |          |        | 83.0 | 12.9   | 0.0   | 43.7  |




# Quantitation Results Report (QT Reviewed)


| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 2,2-Dichloropropane | 131.4031 | 5.19 | -0.01    | 150902 | 41.0 | 63.6   | 36.5  | 96.5  |
|                     |          |      |          |        | 97.0 | 22.5   | 0.0   | 53.2  |

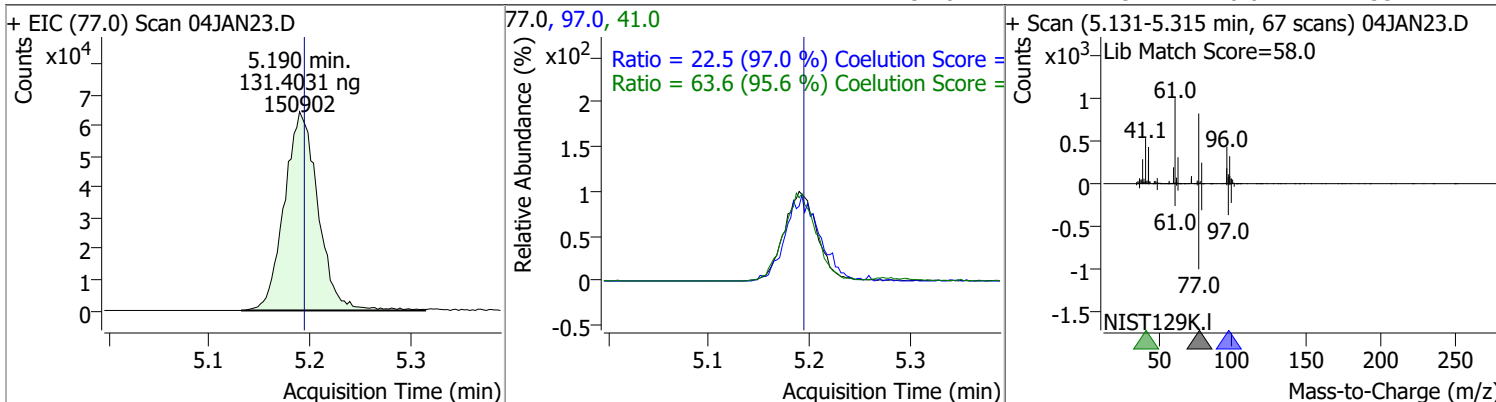


| Compound               | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,2-Dichloroethene | 130.1231 | 5.21 | -0.01    | 108623 | 61.0 | 168.1  | 137.2 | 197.2 |
|                        |          |      |          |        | 98.0 | 67.7   | 37.3  | 97.3  |

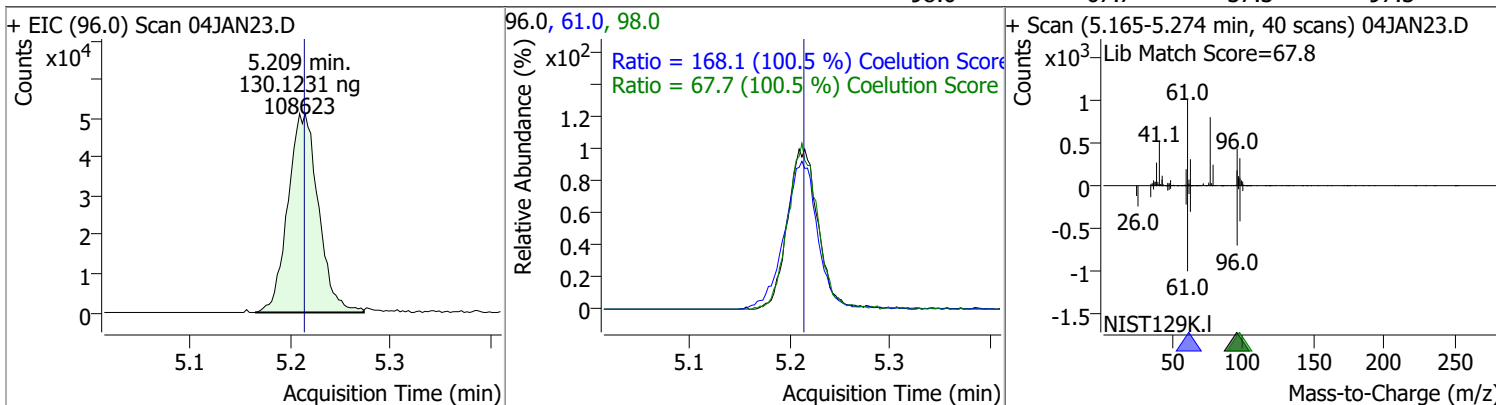

| Compound            | Conc.     | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|-----------|------|----------|--------|------|--------|-------|-------|
| Methyl ethyl ketone | 1198.4439 | 5.28 | 0.00     | 135511 | 72.0 | 20.4   | 0.0   | 51.3  |



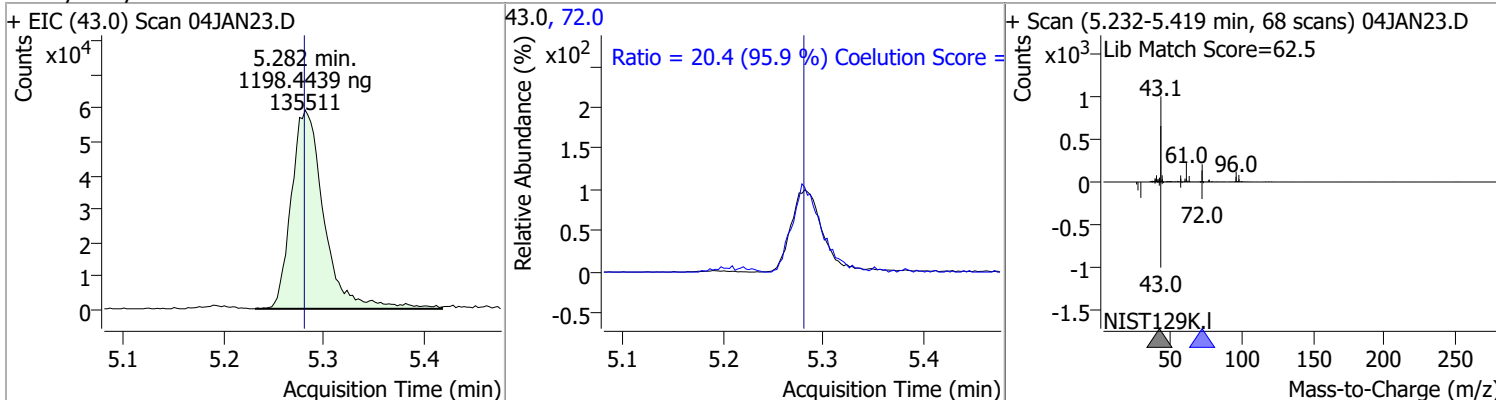


| Compound           | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|-------|------|--------|-------|-------|
| Bromochloromethane | 123.6009 | 5.51 | -0.01    | 42744 | 49.0 | 184.6  | 152.9 | 212.9 |



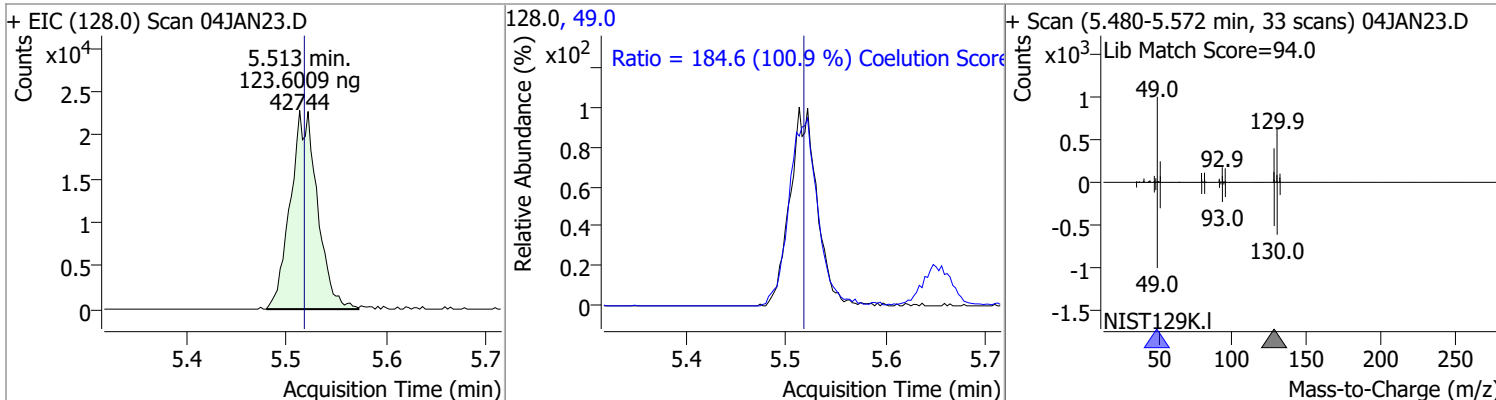


# Quantitation Results Report (QT Reviewed)




| Compound   | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|------|--------|-------|-------|
| Chloroform | 120.4236 | 5.65 | -0.01    | 183676 | 85.0 | 66.1   | 36.0  | 96.0  |






| Compound              | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1,1-Trichloroethane | 128.2524 | 5.83 | 0.00     | 183324 | 99.0 | 65.1   | 34.7  | 94.7  |
|                       |          |      |          |        | 61.0 | 48.9   | 18.1  | 78.1  |



| Compound             | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Dibromofluoromethane | 271.1994 | 5.85 | 0.00     | 204707 | 191.5 | 22.0   | 0.0   | 53.1  |




| Compound             | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Carbon tetrachloride | 128.7928 | 6.03 | 0.00     | 181384 | 119.0 | 96.4   | 67.2  | 127.2 |
|                      |          |      |          |        | 121.0 | 30.9   | 0.1   | 60.1  |




# Quantitation Results Report (QT Reviewed)


| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|-------|--------|-------|-------|
| 1,1-Dichloropropene | 124.1853 | 6.04 | 0.00     | 150930 | 110.0 | 36.1   | 5.9   | 65.9  |
|                     |          |      |          |        | 77.0  | 30.4   | 0.1   | 60.1  |

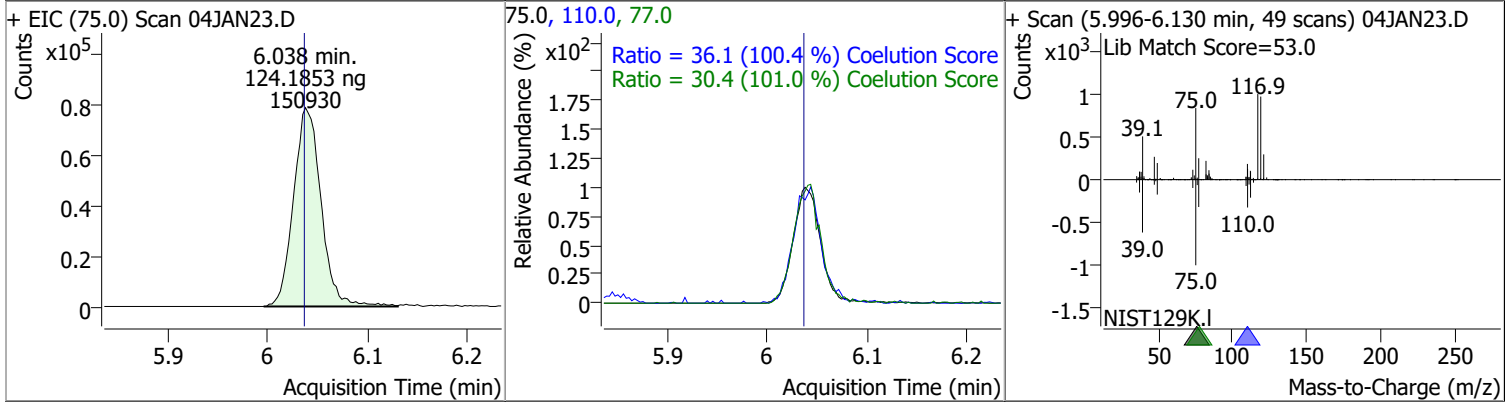


| Compound              | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 280.2886 | 6.23 | 0.00     | 91382 | 65.0 | 194.9  | 166.5 | 226.5 |

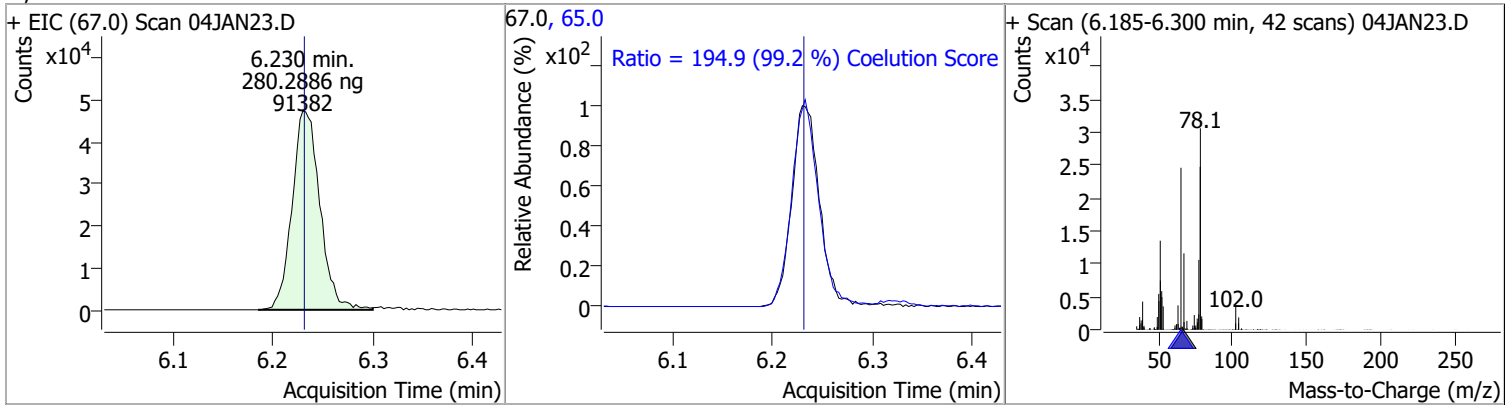

| Compound | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|----------|----------|------|----------|--------|------|--------|-------|-------|
| Benzene  | 131.3139 | 6.28 | 0.00     | 418900 | 77.0 | 23.2   | 0.0   | 53.5  |

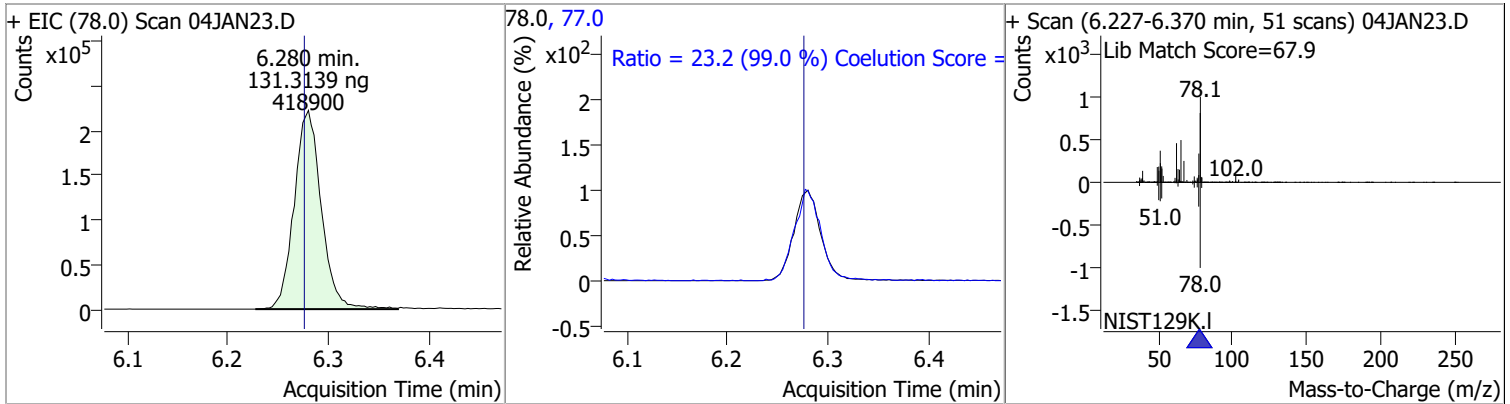


| Compound           | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloroethane | 120.7991 | 6.32 | 0.00     | 104249 | 64.0 | 33.3   | 0.0   | 59.9  |
|                    |          |      |          |        | 98.0 | 8.1    | 0.0   | 37.6  |

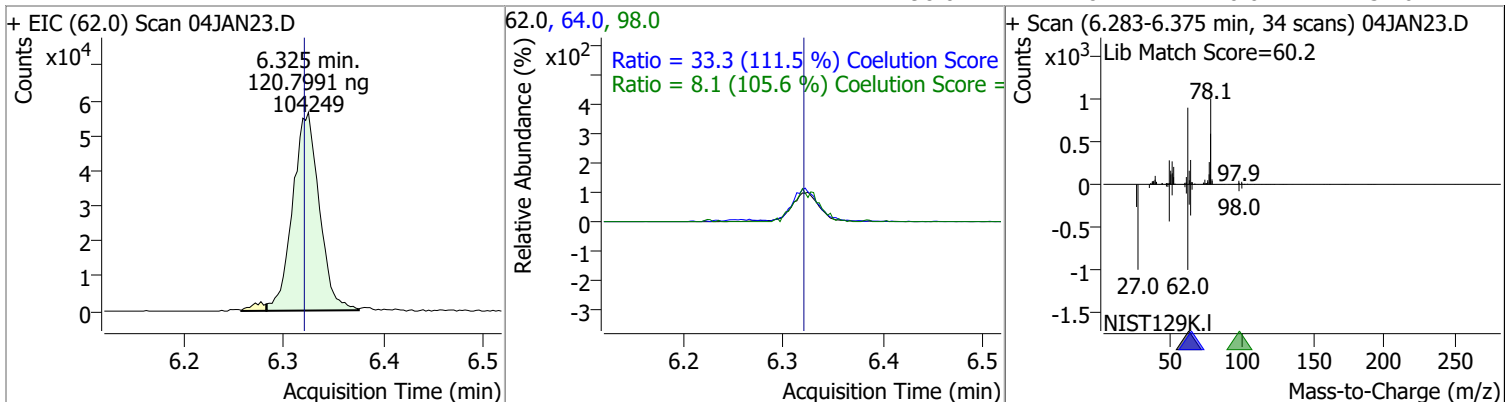




# Quantitation Results Report (QT Reviewed)


| Compound        | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|-----------------|----------|------|----------|--------|-------|--------|-------|-------|
| Trichloroethene | 131.1096 | 7.02 | -0.01    | 121734 | 130.0 | 102.3  | 71.5  | 131.5 |
|                 |          |      |          |        | 97.0  | 63.0   | 34.1  | 94.1  |



| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloropropane | 125.6626 | 7.27 | 0.00     | 102633 | 76.0 | 37.9   | 8.2   | 68.2  |




| Compound       | Conc.    | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|----------------|----------|------|----------|-------|-------|--------|-------|-------|
| Dibromomethane | 125.3047 | 7.39 | -0.01    | 43248 | 173.5 | 109.3  | 83.7  | 143.7 |
|                |          |      |          |       | 95.0  | 81.2   | 52.2  | 112.2 |




# Quantitation Results Report (QT Reviewed)


| Compound             | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Bromodichloromethane | 128.8759 | 7.59 | 0.00     | 122757 | 85.0  | 64.3   | 34.5  | 94.5  |
|                      |          |      |          |        | 127.0 | 9.3    | 0.0   | 39.6  |

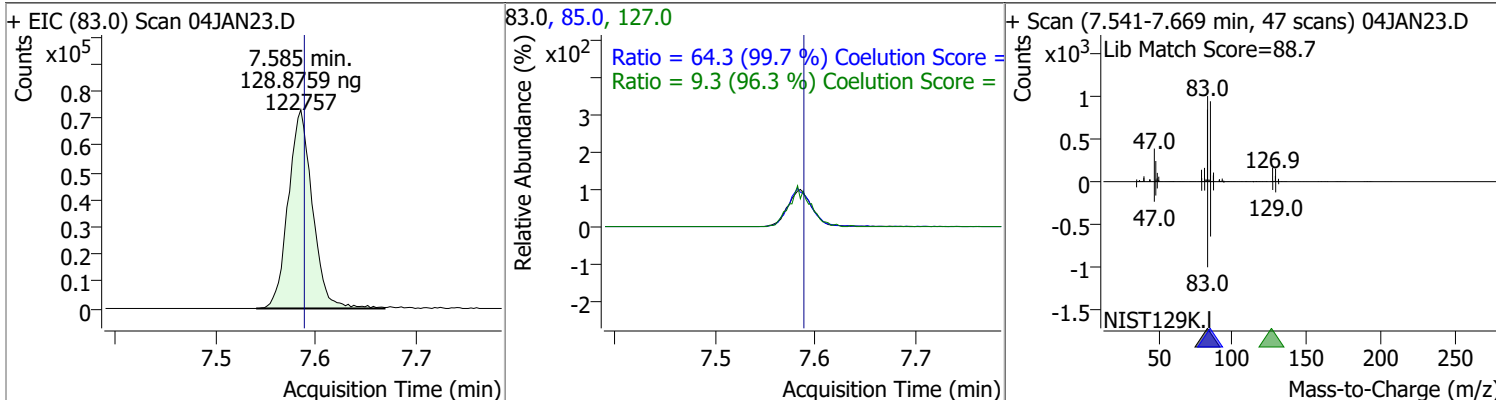

| Compound                | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|-------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,3-Dichloropropene | 121.5561 | 8.05 | -0.01    | 130910 | 39.0 | 51.6   | 23.3  | 83.3  |
|                         |          |      |          |        | 77.0 | 31.2   | 1.0   | 61.0  |

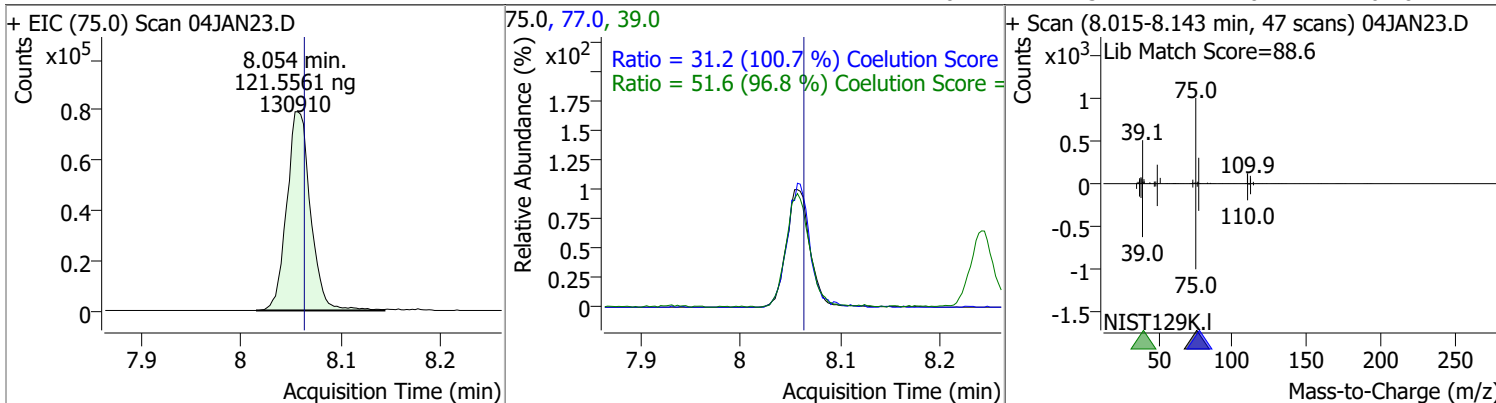


| Compound   | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 276.9106 | 8.32 | 0.00     | 821531 | 100.0 | 64.3   | 34.4  | 94.4  |
|            |          |      |          |        | 99.0  | 9.6    | 0.0   | 39.6  |

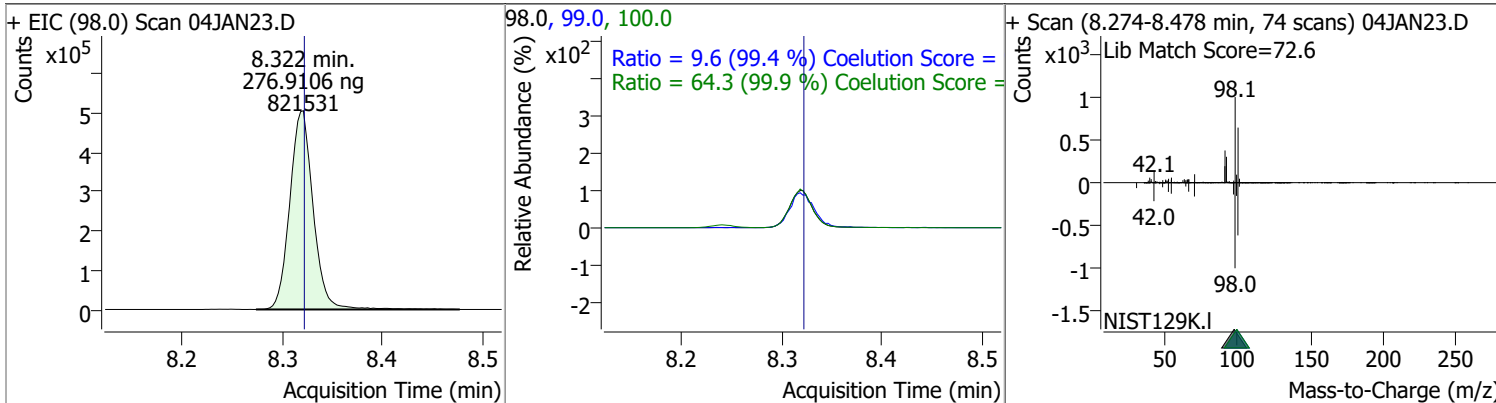


# Quantitation Results Report (QT Reviewed)


| Compound | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|----------|----------|------|----------|--------|------|--------|-------|-------|
| Toluene  | 132.0244 | 8.39 | 0.00     | 264584 | 91.0 | 175.5  | 145.8 | 205.8 |















| Compound                  | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|----------|------|----------|-------|------|--------|-------|-------|
| trans-1,3-Dichloropropene | 129.0216 | 8.64 | 0.00     | 98907 | 39.0 | 50.5   | 23.4  | 83.4  |
|                           |          |      |          |       | 77.0 | 31.0   | 2.4   | 62.4  |

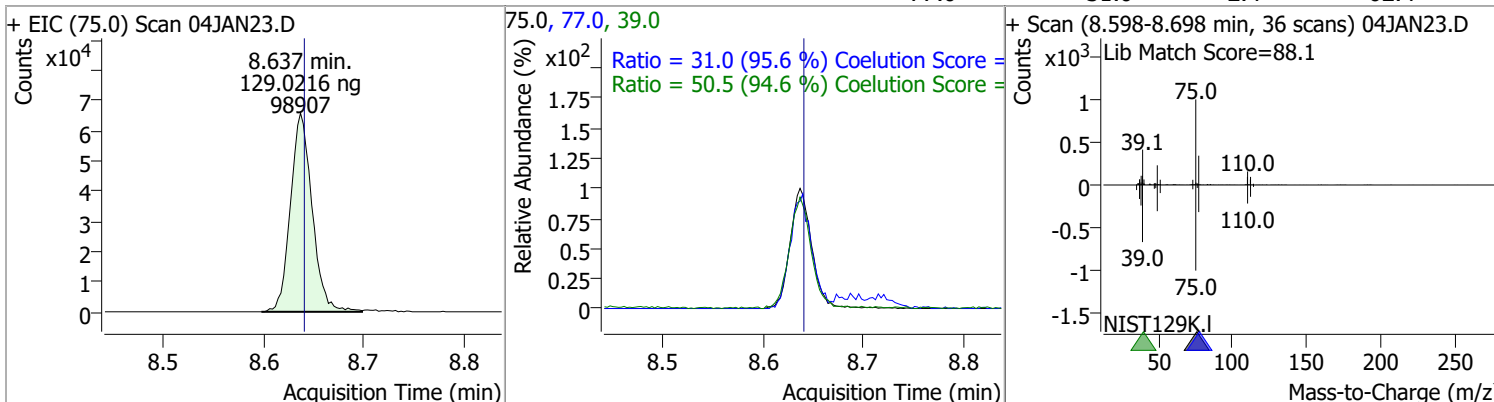





| Compound              | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,1,2-Trichloroethane | 123.0361 | 8.82 | 0.00     | 49128 | 97.0 | 115.4  | 84.6  | 144.6 |
|                       |          |      |          |       | 85.0 | 64.6   | 37.6  | 97.6  |

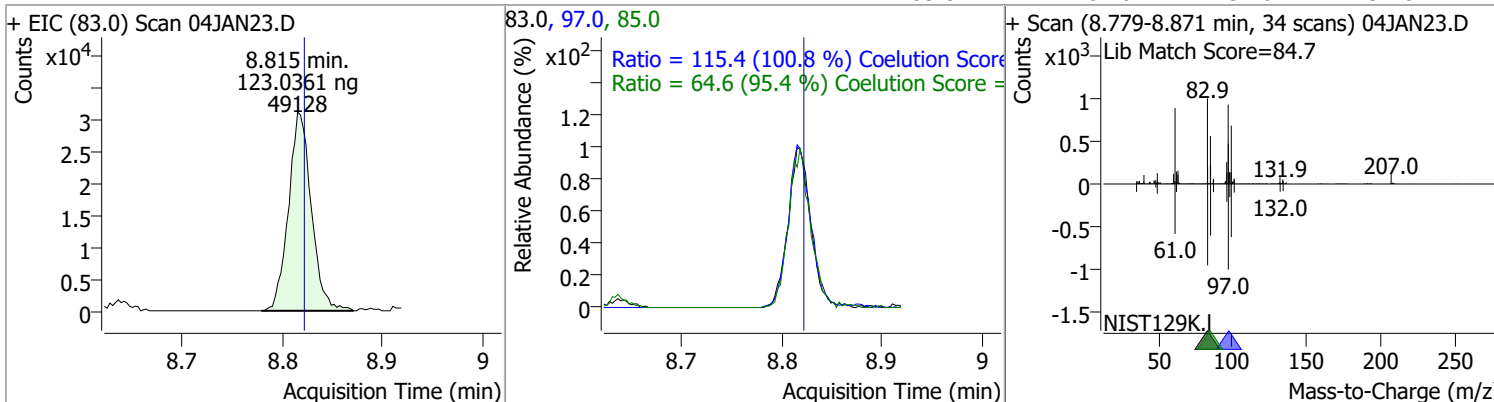

# Quantitation Results Report (QT Reviewed)

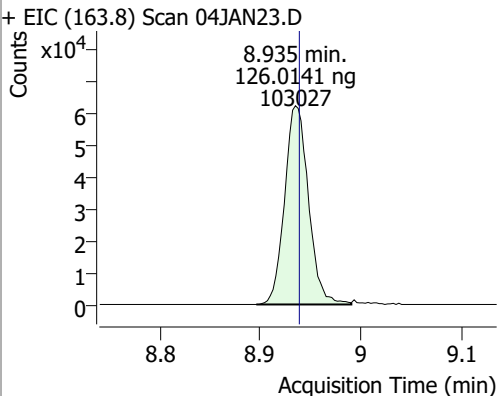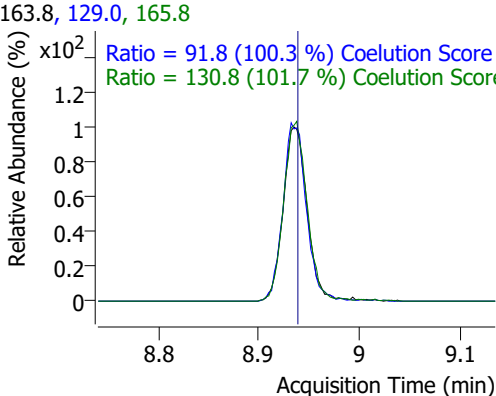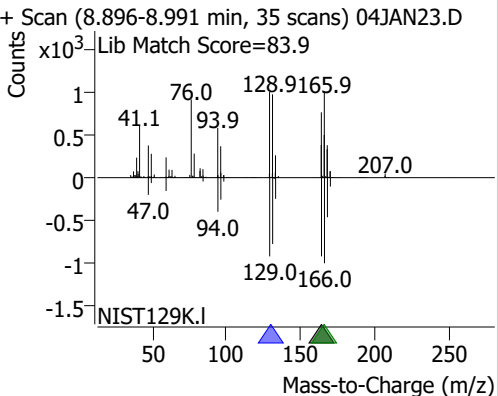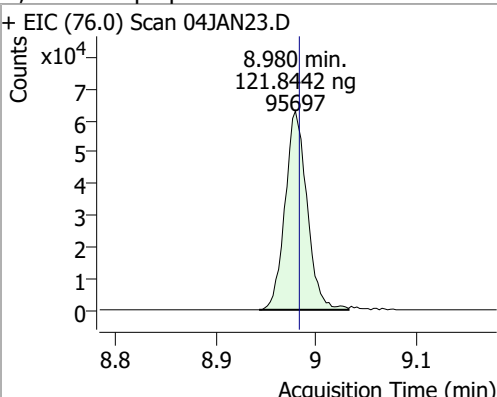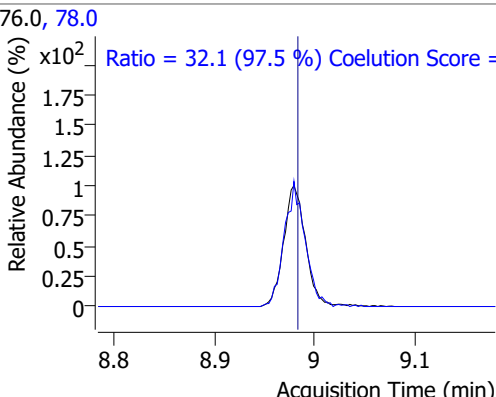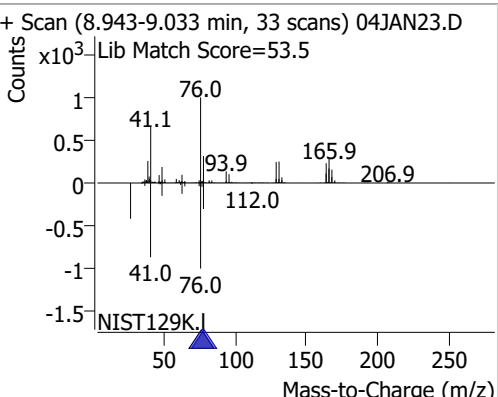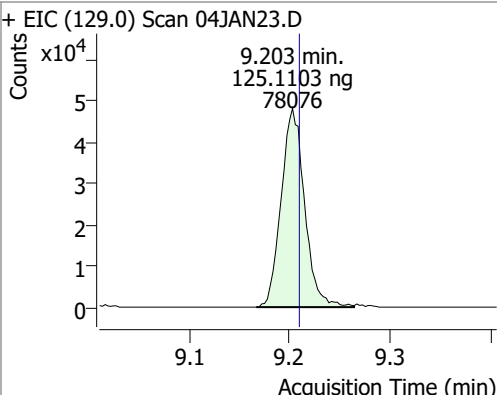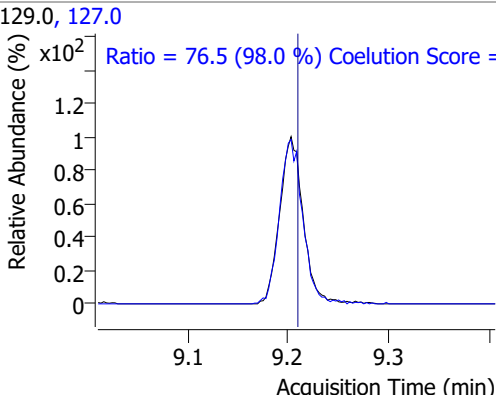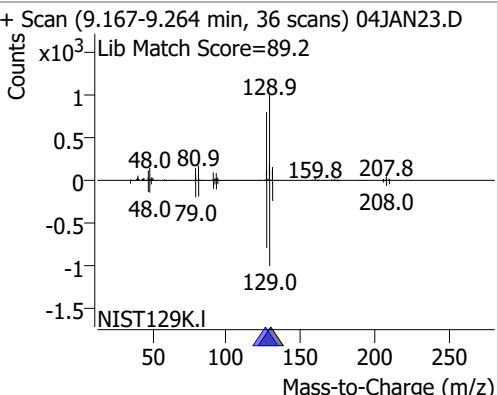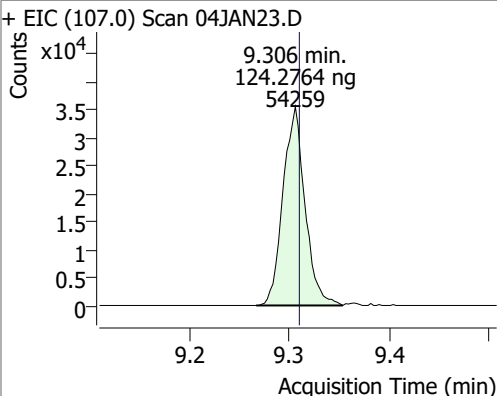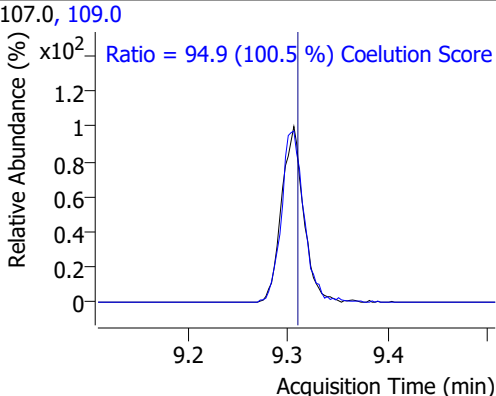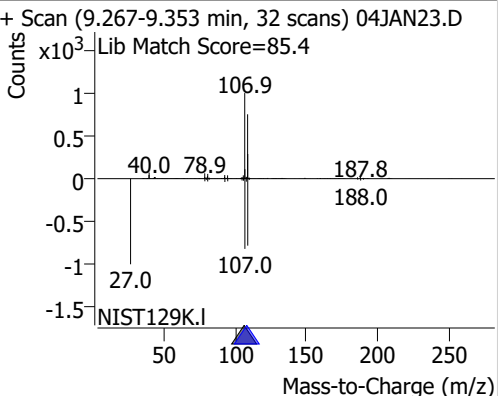
| Compound                                                                           | Conc.                               | RT   | Dev(Min)                                                                             | Resp.                                                                                 | QIon           | QRatio                                                                                | Lower        | Upper          |
|------------------------------------------------------------------------------------|-------------------------------------|------|--------------------------------------------------------------------------------------|---------------------------------------------------------------------------------------|----------------|---------------------------------------------------------------------------------------|--------------|----------------|
| Tetrachloroethene                                                                  | 126.0141                            | 8.94 | 0.00                                                                                 | 103027                                                                                | 165.8<br>129.0 | 130.8<br>91.8                                                                         | 98.6<br>61.5 | 158.6<br>121.5 |
| + EIC (163.8) Scan 04JAN23.D                                                       |                                     |      | 163.8, 129.0, 165.8                                                                  |                                                                                       |                | + Scan (8.896-8.991 min, 35 scans) 04JAN23.D                                          |              |                |
|    | 8.935 min.<br>126.0141 ng<br>103027 |      |    | Ratio = 91.8 (100.3 %) Coelution Score =<br>Ratio = 130.8 (101.7 %) Coelution Score = |                |    |              |                |
| 1,3-Dichloropropane                                                                | 121.8442                            | 8.98 | 0.00                                                                                 | 95697                                                                                 | 78.0           | 32.1                                                                                  | 2.9          | 62.9           |
| + EIC (76.0) Scan 04JAN23.D                                                        |                                     |      | 76.0, 78.0                                                                           |                                                                                       |                | + Scan (8.943-9.033 min, 33 scans) 04JAN23.D                                          |              |                |
|   | 8.980 min.<br>121.8442 ng<br>95697  |      |   | Ratio = 32.1 (97.5 %) Coelution Score =                                               |                |   |              |                |
| Chlorodibromomethane                                                               | 125.1103                            | 9.20 | 0.00                                                                                 | 78076                                                                                 | 127.0          | 76.5                                                                                  | 48.0         | 108.0          |
| + EIC (129.0) Scan 04JAN23.D                                                       |                                     |      | 129.0, 127.0                                                                         |                                                                                       |                | + Scan (9.167-9.264 min, 36 scans) 04JAN23.D                                          |              |                |
|  | 9.203 min.<br>125.1103 ng<br>78076  |      |  | Ratio = 76.5 (98.0 %) Coelution Score =                                               |                |  |              |                |
| 1,2-Dibromoethane                                                                  | 124.2764                            | 9.31 | 0.00                                                                                 | 54259                                                                                 | 109.0          | 94.9                                                                                  | 64.5         | 124.5          |
| + EIC (107.0) Scan 04JAN23.D                                                       |                                     |      | 107.0, 109.0                                                                         |                                                                                       |                | + Scan (9.267-9.353 min, 32 scans) 04JAN23.D                                          |              |                |
|  | 9.306 min.<br>124.2764 ng<br>54259  |      |  | Ratio = 94.9 (100.5 %) Coelution Score =                                              |                |  |              |                |

# Quantitation Results Report (QT Reviewed)




# Quantitation Results Report (QT Reviewed)


| Compound | Conc.    | RT    | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|----------|----------|-------|----------|--------|------|--------|-------|-------|
| o-Xylene | 132.2214 | 10.43 | 0.00     | 174061 | 91.0 | 215.8  | 183.1 | 243.1 |

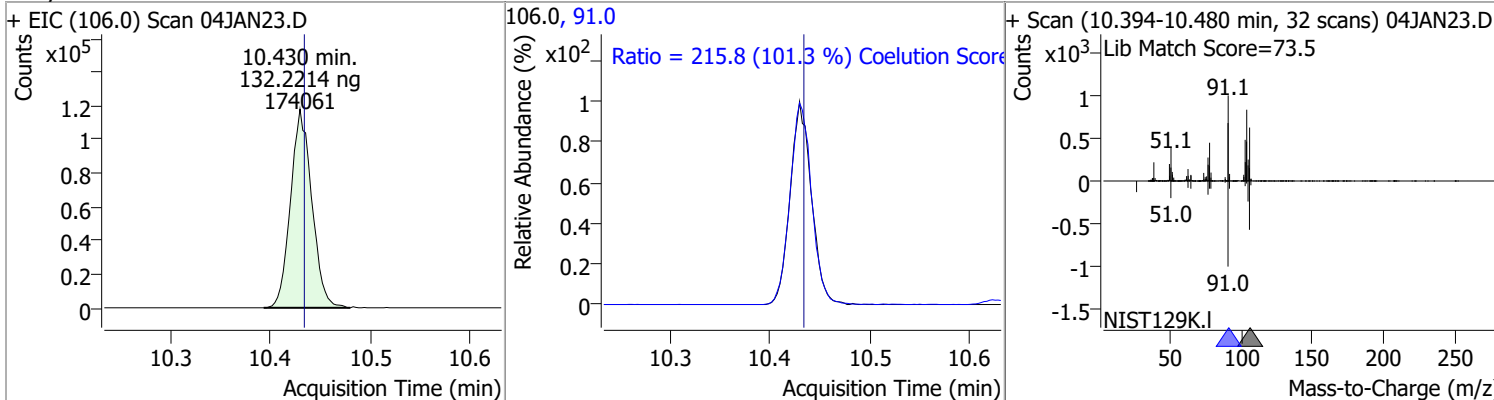


| Compound | Conc.    | RT    | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|----------|----------|-------|----------|--------|------|--------|-------|-------|
| Styrene  | 137.4974 | 10.45 | 0.00     | 291425 | 78.0 | 48.1   | 19.6  | 79.6  |

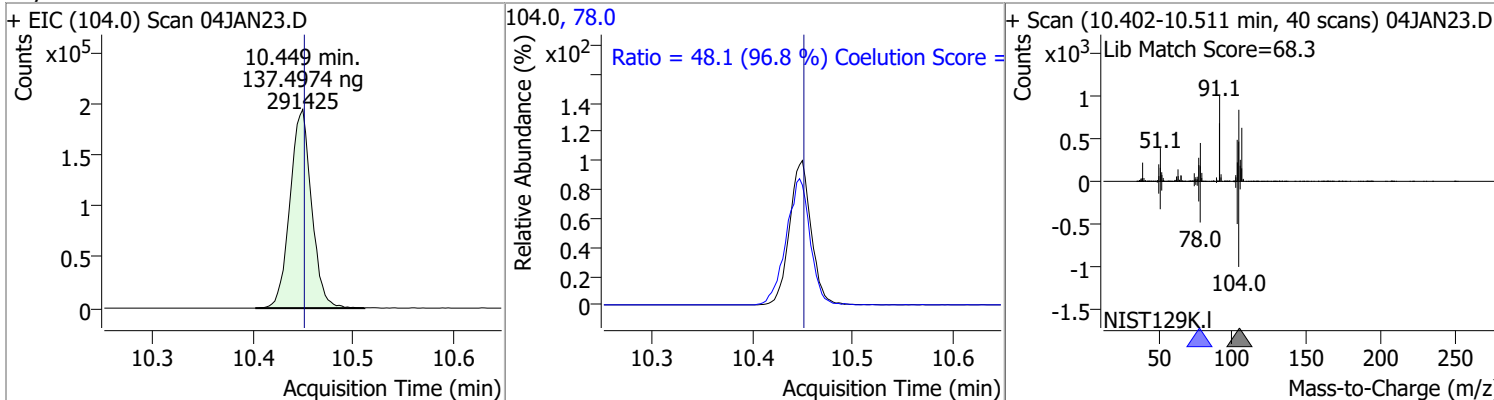

| Compound  | Conc.    | RT    | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|-----------|----------|-------|----------|-------|-------|--------|-------|-------|
| Bromoform | 129.9644 | 10.63 | 0.00     | 42560 | 170.5 | 50.3   | 22.1  | 82.1  |
|           |          |       |          |       | 174.5 | 49.3   | 20.1  | 80.1  |

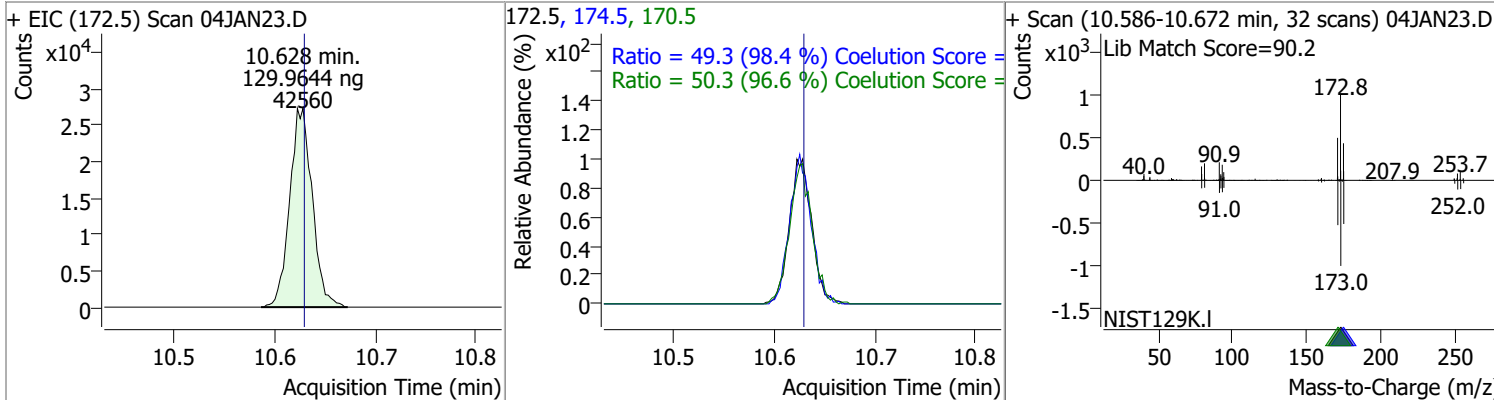


| Compound             | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 269.8976 | 10.95 | 0.00     | 253034 | 174.0 | 93.4   | 61.7  | 121.7 |
|                      |          |       |          |        | 176.0 | 90.2   | 60.6  | 120.6 |

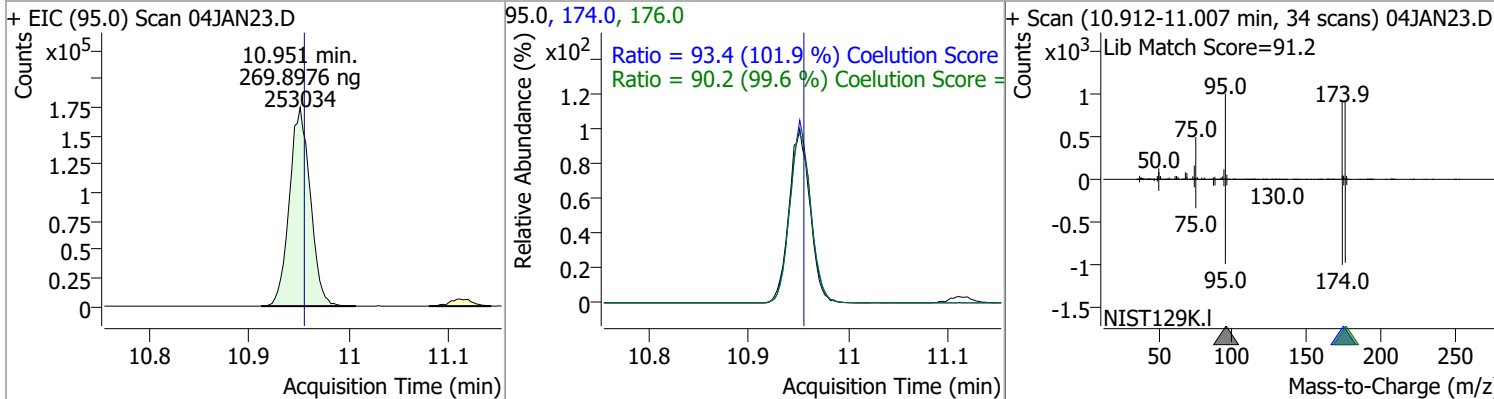


# Quantitation Results Report (QT Reviewed)


| Compound     | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|--------------|----------|-------|----------|--------|-------|--------|-------|-------|
| Bromobenzene | 131.6788 | 11.09 | 0.00     | 109054 | 77.0  | 146.1  | 115.7 | 175.7 |
|              |          |       |          |        | 158.0 | 99.0   | 66.5  | 126.5 |

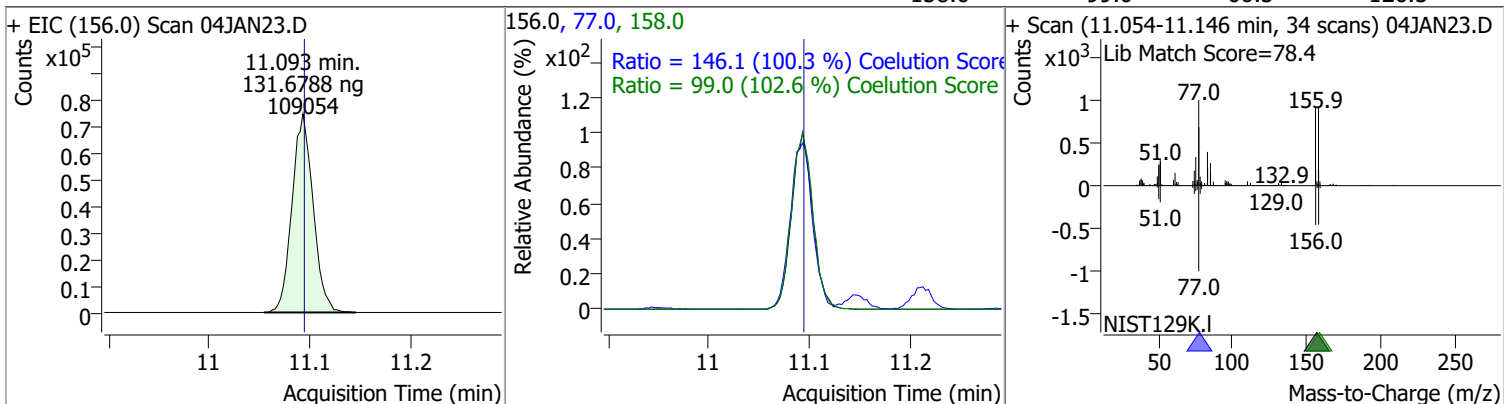


| Compound                  | Conc.    | RT    | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|----------|-------|----------|-------|------|--------|-------|-------|
| 1,1,2,2-Tetrachloroethane | 127.4722 | 11.11 | 0.00     | 60763 | 85.0 | 64.8   | 36.2  | 96.2  |

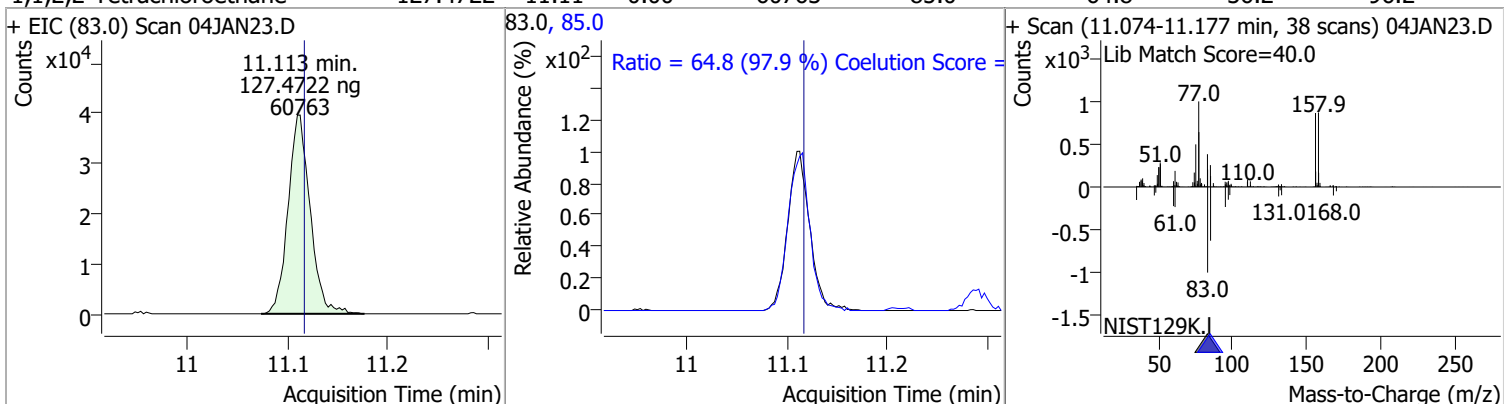

| Compound               | Conc.    | RT    | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|------------------------|----------|-------|----------|-------|-------|--------|-------|-------|
| 1,2,3-Trichloropropane | 122.9523 | 11.15 | 0.00     | 15682 | 112.0 | 62.6   | 33.5  | 93.5  |



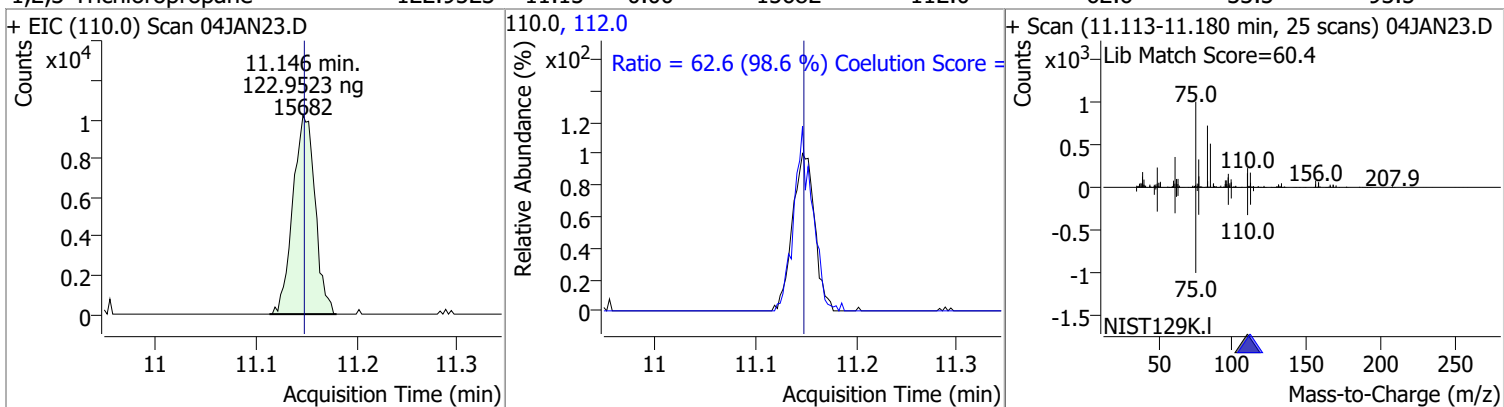


| Compound        | Conc.    | RT    | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|-----------------|----------|-------|----------|--------|------|--------|-------|-------|
| 2-Chlorotoluene | 131.2948 | 11.29 | 0.00     | 108192 | 91.0 | 290.9  | 252.3 | 312.3 |



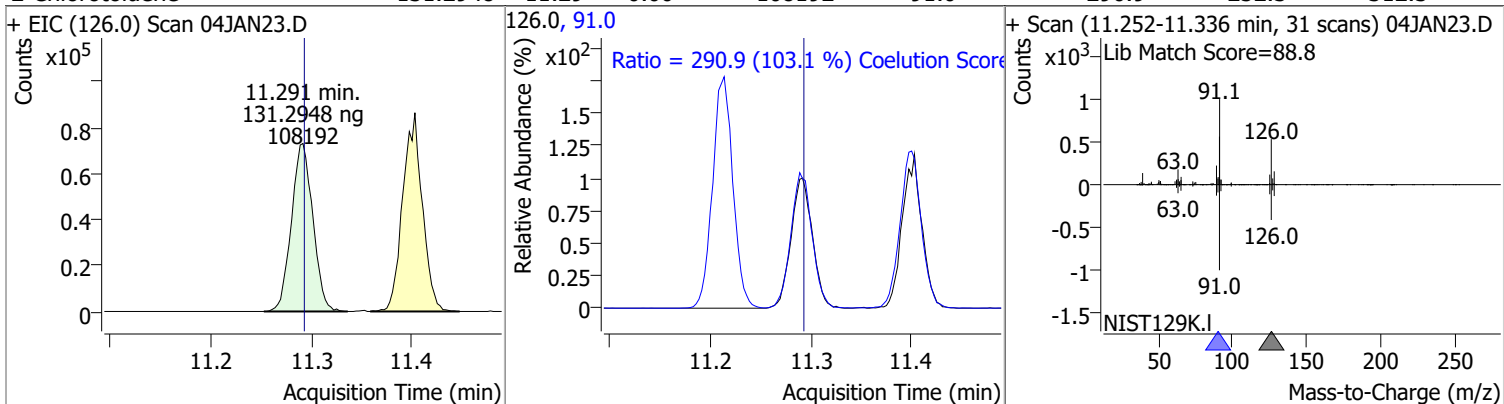


# Quantitation Results Report (QT Reviewed)




| Compound        | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|-----------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 4-Chlorotoluene | 137.0790 | 11.40 | 0.00     | 368295 | 126.0 | 31.8   | 1.7   | 61.7  |

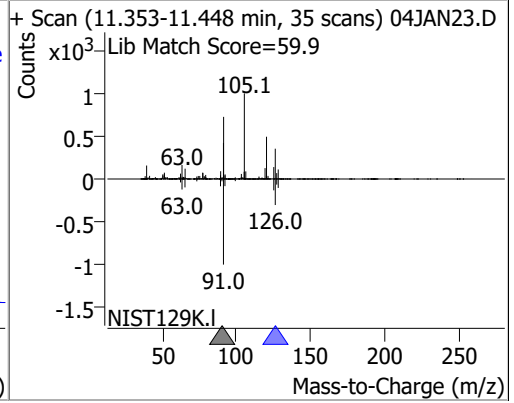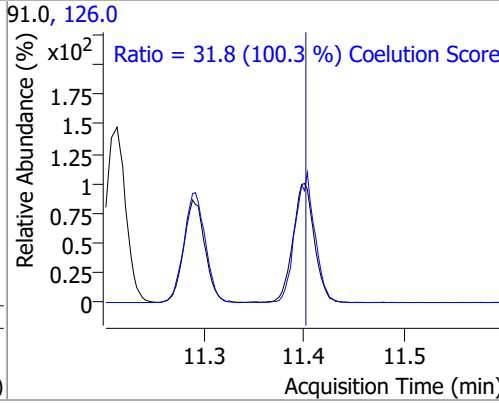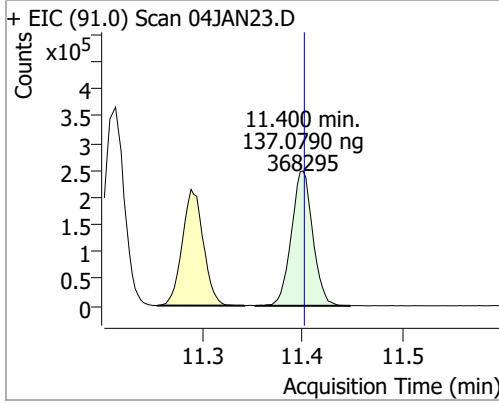

| Compound            | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,3-Dichlorobenzene | 135.1185 | 12.03 | 0.00     | 204088 | 148.0 | 63.2   | 33.6  | 93.6  |
|                     |          |       |          |        | 111.0 | 38.4   | 9.8   | 69.8  |

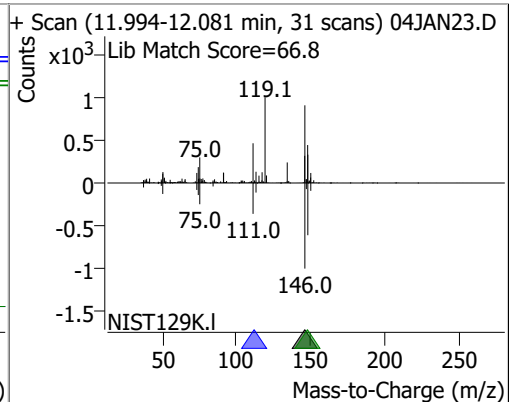




| Compound            | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,4-Dichlorobenzene | 129.8812 | 12.12 | 0.00     | 200032 | 148.0 | 63.9   | 33.1  | 93.1  |
|                     |          |       |          |        | 111.0 | 39.1   | 9.1   | 69.1  |

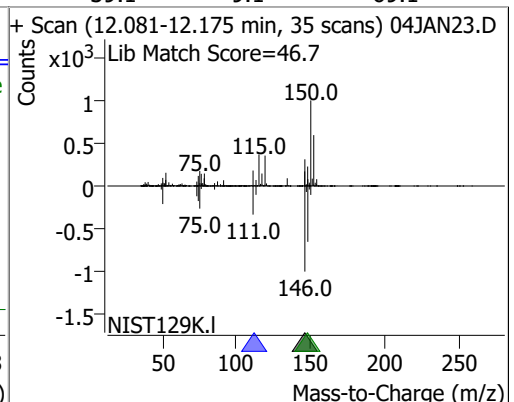



# Quantitation Results Report (QT Reviewed)

| Compound            | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,2-Dichlorobenzene | 128.7104 | 12.49 | 0.00     | 164299 | 148.0 | 64.3   | 33.9  | 93.9  |
|                     |          |       |          |        | 111.0 | 40.6   | 11.0  | 71.0  |

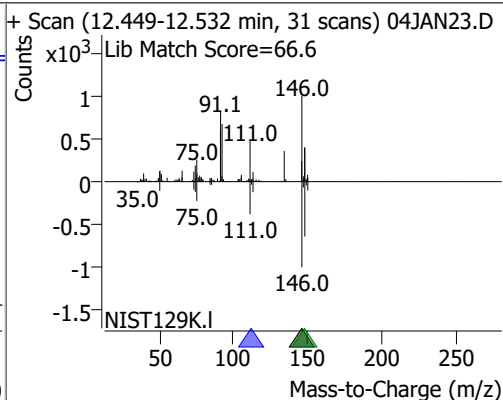

# Audit Trail report

**Batch name and path:** D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422\_8260B.batch.bin  
**Quant batch version:** 10.0  
**Quant reporting version:** 10.0

| Name                         | User           | Time                 | Action                                                                                                            | Reason | Comment | Succeed | Exception |
|------------------------------|----------------|----------------------|-------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdNewBatchTable             | BL2000\mchavez | 1/4/2022 10:36:43 AM | Create new batch<br>D:\Org\Data\VOA5975C\VG010422\VG010422_8260B.batch.bin                                        |        |         | ✓       |           |
| CmdImportSamplesFromWorklist | BL2000\mchavez | 1/4/2022 10:36:56 AM | Add samples from worklist:<br>D:\Org\Data\VOA5975C\VG010422\04JAN02.D,<br>D:\Org\Data\VOA5975C\VG010422\04JAN01.D |        |         | ✓       |           |
| CmdSetSampleAttribute        | BL2000\mchavez | 1/4/2022 10:37:01 AM | Set SampleType = MatrixBlank for sample 04JAN02.D; previous value = Sample                                        |        |         | ✓       |           |
| CmdSetSampleAttribute        | BL2000\mchavez | 1/4/2022 10:37:04 AM | Set SampleType = TuneCheck for sample 04JAN02.D; previous value = MatrixBlank                                     |        |         | ✓       |           |
| CmdStartMethodEditing        | BL2000\mchavez | 1/4/2022 10:52:58 AM | Start method editing                                                                                              |        |         | ✓       |           |
| CmdImportMethodFromBatch     | BL2000\mchavez | 1/4/2022 10:52:59 AM | Import method from batch<br>D:\Org\Data\VOA5975C\VG010322\VG010322_8260B_2ndRun.batch.bin                         |        |         | ✓       |           |
| CmdApplyMethodToAllSamples   | BL2000\mchavez | 1/4/2022 10:53:03 AM | Apply method to all samples                                                                                       |        |         | ✓       |           |
| CmdMethodClear               | BL2000\mchavez | 1/4/2022 10:53:03 AM | Clear method                                                                                                      |        |         | ✓       |           |
| CmdEndMethodEditing          | BL2000\mchavez | 1/4/2022 10:53:03 AM | End method editing                                                                                                |        |         | ✓       |           |
| CmdQuantitate                | BL2000\mchavez | 1/4/2022 10:53:07 AM | Quantitate all compounds in all samples                                                                           |        |         | ✓       |           |
| CmdSaveBatchTable            | BL2000\mchavez | 1/4/2022 10:54:55 AM | Save batch<br>D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin                                 |        |         | ✓       |           |
| CmdOpenBatchTable            | BL2000\mchavez | 1/4/2022 11:14:07 AM | Open batch<br>D:\Org\Data\VOA5975C\VG010422\VG010422_8260B.batch.bin                                              |        |         | ✓       |           |
| CmdImportSamplesFromWorklist | BL2000\mchavez | 1/4/2022 11:14:24 AM | Add samples from worklist:<br>D:\Org\Data\VOA5975C\VG010422\04JAN03.D                                             |        |         | ✓       |           |
| CmdSetSampleAttribute        | BL2000\mchavez | 1/4/2022 11:14:28 AM | Set SampleType = CC for sample 04JAN03.D; previous value = Sample                                                 |        |         | ✓       |           |
| CmdSetSampleAttribute        | BL2000\mchavez | 1/4/2022 11:14:31 AM | Set LevelName = CC for sample 04JAN03.D; previous value =                                                         |        |         | ✓       |           |
| CmdQuantitate                | BL2000\mchavez | 1/4/2022 11:14:35 AM | Quantitate all compounds in all samples                                                                           |        |         | ✓       |           |
| CmdSaveBatchTable            | BL2000\mchavez | 1/4/2022 11:15:38 AM | Save batch<br>D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin                                 |        |         | ✓       |           |
| CmdOpenBatchTable            | BL2000\mchavez | 1/4/2022 1:02:39 PM  | Open batch<br>D:\Org\Data\VOA5975C\VG010422\VG010422_8260B.batch.bin                                              |        |         | ✓       |           |

# Audit Trail report

| Name                         | User           | Time                | Action                                                                                                            | Reason | Comment | Succeed | Exception |
|------------------------------|----------------|---------------------|-------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdImportSamplesFromWorklist | BL2000\mchavez | 1/4/2022 1:02:58 PM | Add samples from worklist:<br>D:\Org\Data\VOA5975C\VG010422\04JAN05.D,<br>D:\Org\Data\VOA5975C\VG010422\04JAN04.D |        |         | ✓       |           |
| CmdSetSampleAttribute        | BL2000\mchavez | 1/4/2022 1:03:09 PM | Set SampleType = TuneCheck for sample 04JAN05.D; previous value = Sample                                          |        |         | ✓       |           |
| CmdQuantitate                | BL2000\mchavez | 1/4/2022 1:03:40 PM | Quantitate all compounds in all samples                                                                           |        |         | ✓       |           |
| CmdSaveBatchTable            | BL2000\mchavez | 1/4/2022 1:14:26 PM | Save batch<br>D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin                                 |        |         | ✓       |           |
| CmdOpenBatchTable            | BL2000\mchavez | 1/4/2022 1:47:13 PM | Open batch<br>D:\Org\Data\VOA5975C\VG010422\VG010422_8260B.batch.bin                                              |        |         | ✓       |           |
| CmdImportSamplesFromWorklist | BL2000\mchavez | 1/4/2022 1:47:29 PM | Add samples from worklist:<br>D:\Org\Data\VOA5975C\VG010422\04JAN06.D                                             |        |         | ✓       |           |
| CmdSetSampleAttribute        | BL2000\mchavez | 1/4/2022 1:47:35 PM | Set SampleType = CC for sample 04JAN06.D; previous value = Sample                                                 |        |         | ✓       |           |
| CmdSetSampleAttribute        | BL2000\mchavez | 1/4/2022 1:47:38 PM | Set LevelName = CC for sample 04JAN06.D; previous value =                                                         |        |         | ✓       |           |
| CmdQuantitate                | BL2000\mchavez | 1/4/2022 1:47:44 PM | Quantitate all compounds in all samples                                                                           |        |         | ✓       |           |
| CmdSaveBatchTable            | BL2000\mchavez | 1/4/2022 1:53:45 PM | Save batch<br>D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin                                 |        |         | ✓       |           |
| CmdOpenBatchTable            | BL2000\mchavez | 1/4/2022 3:05:35 PM | Open batch<br>D:\Org\Data\VOA5975C\VG010422\VG010422_8260B.batch.bin                                              |        |         | ✓       |           |
| CmdImportSamplesFromWorklist | BL2000\mchavez | 1/4/2022 3:06:14 PM | Add samples from worklist:<br>D:\Org\Data\VOA5975C\VG010422\04JAN08.D,<br>D:\Org\Data\VOA5975C\VG010422\04JAN07.D |        |         | ✓       |           |
| CmdSetSampleAttribute        | BL2000\mchavez | 1/4/2022 3:06:26 PM | Set SampleType = TuneCheck for sample 04JAN08.D; previous value = Sample                                          |        |         | ✓       |           |
| CmdSaveBatchTable            | BL2000\mchavez | 1/4/2022 3:24:14 PM | Save batch<br>D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin                                 |        |         | ✓       |           |
| CmdOpenBatchTable            | BL2000\mchavez | 1/5/2022 8:56:03 AM | Open batch<br>D:\Org\Data\VOA5975C\VG010422\VG010422_8260B.batch.bin                                              |        |         | ✓       |           |

# Audit Trail report

| Name                         | User           | Time                | Action                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                    | Reason | Comment | Succeed | Exception |
|------------------------------|----------------|---------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdImportSamplesFromWorklist | BL2000\mchavez | 1/5/2022 8:58:43 AM | Add samples from worklist:<br>D:\Org\Data\VOA5975C\VG010422\04JAN28.D,<br>D:\Org\Data\VOA5975C\VG010422\04JAN27.D,<br>D:\Org\Data\VOA5975C\VG010422\04JAN26.D,<br>D:\Org\Data\VOA5975C\VG010422\04JAN25.D,<br>D:\Org\Data\VOA5975C\VG010422\04JAN24.D,<br>D:\Org\Data\VOA5975C\VG010422\04JAN23.D,<br>D:\Org\Data\VOA5975C\VG010422\04JAN22.D,<br>D:\Org\Data\VOA5975C\VG010422\04JAN21.D,<br>D:\Org\Data\VOA5975C\VG010422\04JAN20.D,<br>D:\Org\Data\VOA5975C\VG010422\04JAN19.D,<br>D:\Org\Data\VOA5975C\VG010422\04JAN18.D,<br>D:\Org\Data\VOA5975C\VG010422\04JAN17.D,<br>D:\Org\Data\VOA5975C\VG010422\04JAN16.D,<br>D:\Org\Data\VOA5975C\VG010422\04JAN15.D,<br>D:\Org\Data\VOA5975C\VG010422\04JAN14.D,<br>D:\Org\Data\VOA5975C\VG010422\04JAN13.D,<br>D:\Org\Data\VOA5975C\VG010422\04JAN12.D,<br>D:\Org\Data\VOA5975C\VG010422\04JAN11.D,<br>D:\Org\Data\VOA5975C\VG010422\04JAN10.D,<br>D:\Org\Data\VOA5975C\VG010422\04JAN09.D |        |         | ✓       |           |
| CmdSetSampleAttribute        | BL2000\mchavez | 1/5/2022 8:59:26 AM | Set SampleType = Blank for sample 04JAN09.D; previous value = Sample                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                      |        |         | ✓       |           |
| CmdSetSampleAttribute        | BL2000\mchavez | 1/5/2022 8:59:31 AM | Set SampleType = Calibration for sample 04JAN10.D; previous value = Sample                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                |        |         | ✓       |           |
| CmdSetSampleAttribute        | BL2000\mchavez | 1/5/2022 8:59:35 AM | Set SampleType = Calibration for sample 04JAN11.D; previous value = Sample                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                |        |         | ✓       |           |
| CmdSetSampleAttribute        | BL2000\mchavez | 1/5/2022 8:59:40 AM | Set SampleType = Calibration for sample 04JAN12.D; previous value = Sample                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                |        |         | ✓       |           |
| CmdSetSampleAttribute        | BL2000\mchavez | 1/5/2022 8:59:45 AM | Set SampleType = Calibration for sample 04JAN13.D; previous value = Sample                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                |        |         | ✓       |           |

# Audit Trail report

| Name                  | User           | Time                | Action                                                                            | Reason | Comment | Succeed | Exception                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                        |
|-----------------------|----------------|---------------------|-----------------------------------------------------------------------------------|--------|---------|---------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 8:59:50 AM | Set SampleType = Calibration for sample 04JAN15.D; previous value = Sample        |        |         | ✓       |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                  |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 8:59:55 AM | Set SampleType = Calibration for sample 04JAN17.D; previous value = Sample        |        |         | ✓       |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                  |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 9:00:00 AM | Set SampleType = Calibration for sample 04JAN19.D; previous value = Sample        |        |         | ✓       |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                  |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 9:00:08 AM | Set SampleType = Calibration for sample 04JAN21.D; previous value = Sample        |        |         | ✓       |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                  |
| CmdSetSampleAttribute | BL2000\mchavez | 1/5/2022 9:00:14 AM | Set SampleType = QC for sample 04JAN23.D; previous value = Sample                 |        |         | ✓       |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                  |
| CmdSaveBatchTable     | BL2000\mchavez | 1/5/2022 9:11:16 AM | Save batch<br>D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin |        |         | ✓       |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                  |
| CmdOpenBatchTable     | BL2000\mchavez | 1/5/2022 9:58:34 AM | Open batch<br>D:\Org\Data\VOA5975C\VG010422\VG010422_8260B.batch.bin              |        |         | ✓       |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                  |
| CmdQuantitate         | BL2000\mchavez | 1/5/2022 9:58:40 AM | Quantitate all compounds in all samples                                           |        |         |         | Agilent.MassSpectrometry.DataAnalysis.Quantitative.ApplicationCommandException: Batch quantitation failed ---><br>Agilent.MassSpectrometry.DataAnalysis.Quantitative.ApplicationCommandException: Sample not validated: Level name is undefined for a Calibration or QC sample.<br>at<br>Agilent.MassSpectrometry.DataAnalysis.Quantitative.Analysis.Batch.ValidateBatchMethod()<br>at<br>Agilent.MassSpectrometry.DataAnalysis.Quantitative.Analysis.Batch.Quantitate()<br>--- End of inner exception stack<br>trace ---<br>at<br>Agilent.MassSpectrometry.DataAnalysis.Quantitative.Analysis.Batch.Quantitate()<br>at<br>Agilent.MassSpectrometry.DataAnalysis.Quantitative.CmdQuantitate.QuantitateBatch(Int16 batchId)<br>at<br>Agilent.MassSpectrometry.CommandModel.CommandHistory.Invoke(ICommand cmd)<br>at<br>Agilent.MassSpectrometry.DataAnalysis.Quantitative.AppCommandContext.Invoke(ICommand cmd) |

# Audit Trail report

| Name                              | User           | Time                 | Action                                                                                                                                                                                                                | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdSetSampleAttribute             | BL2000\mchavez | 1/5/2022 10:06:05 AM | Set LevelName = 1 for sample 04JAN10.D; previous value =                                                                                                                                                              |        |         | ✓       |           |
| CmdSaveBatchTable                 | BL2000\mchavez | 1/5/2022 10:06:09 AM | Save batch<br>D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin                                                                                                                                     |        |         | ✓       |           |
| CmdOpenBatchTable                 | BL2000\mchavez | 1/5/2022 10:14:38 AM | Open batch<br>D:\Org\Data\VOA5975C\VG010422\VG010422_8260B.batch.bin                                                                                                                                                  |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/5/2022 10:14:47 AM | Set LevelName = 2 for sample 04JAN11.D; previous value =                                                                                                                                                              |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/5/2022 10:14:52 AM | Set LevelName = 3 for sample 04JAN12.D; previous value =                                                                                                                                                              |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/5/2022 10:14:57 AM | Set LevelName = 4 for sample 04JAN13.D; previous value =                                                                                                                                                              |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/5/2022 10:15:05 AM | Set LevelName = 5 for sample 04JAN15.D; previous value =                                                                                                                                                              |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/5/2022 10:15:11 AM | Set LevelName = 6 for sample 04JAN17.D; previous value =                                                                                                                                                              |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/5/2022 10:15:16 AM | Set LevelName = 7 for sample 04JAN19.D; previous value =                                                                                                                                                              |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/5/2022 10:15:21 AM | Set LevelName = 8 for sample 04JAN21.D; previous value =                                                                                                                                                              |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/5/2022 10:15:29 AM | Set LevelName = QC for sample 04JAN23.D; previous value =                                                                                                                                                             |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/5/2022 10:15:36 AM | Set SampleInformation = LCSA for sample 04JAN23.D; previous value =                                                                                                                                                   |        |         | ✓       |           |
| CmdQuantitate                     | BL2000\mchavez | 1/5/2022 10:16:01 AM | Quantitate all compounds in all samples                                                                                                                                                                               |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/5/2022 10:16:49 AM | Manually integrate compound Chloroethane in sample 04JAN10.D, from x, y = 1.874, 1384 to 1.916, 1542, result = 2178; previous integration is from x, y = 1.894, 1143 to 1.933, 1143 and previous response = 2132.     |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:16:53 AM | Manually integrate qualifier 66.0 of compound Chloroethane in sample 04JAN10.D from x, y = 1.869, 0 to 1.908, 8; result = 781                                                                                         |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:16:54 AM | Manually integrate qualifier 66.0 of compound Chloroethane in sample 04JAN10.D, from x, y = 1.869, 0 to 1.913, 0, result = 824; previous integration is from x, y = 1.869, 0 to 1.908, 8 and previous response = 781. |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/5/2022 10:17:08 AM | Manually integrate compound Bromomethane in sample 04JAN10.D from x, y = 1.768, -2 to 1.849, 0; result = 1902                                                                                                         |        |         | ✓       |           |

# Audit Trail report

| Name                              | User           | Time                 | Action                                                                                                                                                                                                                            | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:17:15 AM | Manually integrate qualifier 87.0 of compound Dichlorodifluoromethane in sample 04JAN10.D from x, y = 1.202, 0 to 1.289, 0; result = 1393                                                                                         |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:17:25 AM | Manually integrate qualifier 52.0 of compound Chloromethane in sample 04JAN10.D from x, y = 1.370, 0 to 1.459, 0; result = 1679                                                                                                   |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:17:55 AM | Manually integrate qualifier 64.0 of compound Vinyl chloride in sample 04JAN10.D, from x, y = 1.492, 6362 to 1.506, 5900, result = 1131; previous integration is from x, y = 1.308, 0 to 1.682, 0 and previous response = 192320. |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/5/2022 10:18:11 AM | Manually integrate compound 1,1-Dichloroethene in sample 04JAN10.D from x, y = 2.636, 0 to 2.747, 0; result = 2084                                                                                                                |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:18:16 AM | Manually integrate qualifier 63.0 of compound 1,1-Dichloroethene in sample 04JAN10.D from x, y = 2.672, 0 to 2.753, 0; result = 1158                                                                                              |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:18:38 AM | Manually integrate qualifier 86.0 of compound Methylene chloride in sample 04JAN10.D from x, y = 3.288, 0 to 3.386, 0; result = 1820                                                                                              |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/5/2022 10:19:27 AM | Manually integrate compound trans-1,2-Dichloroethene in sample 04JAN10.D from x, y = 3.673, 0 to 3.762, 0; result = 2146                                                                                                          |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:19:31 AM | Manually integrate qualifier 98.0 of compound trans-1,2-Dichloroethene in sample 04JAN10.D from x, y = 3.684, 0 to 3.779, 0; result = 1426                                                                                        |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/5/2022 10:19:36 AM | Manually integrate compound Methyl tert-butyl ether (MTBE) in sample 04JAN10.D from x, y = 3.698, 0 to 3.832, 0; result = 2717                                                                                                    |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:19:38 AM | Manually integrate qualifier 57.0 of compound Methyl tert-butyl ether (MTBE) in sample 04JAN10.D from x, y = 3.690, 0 to 3.798, 0; result = 531                                                                                   |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/5/2022 10:19:46 AM | Manually integrate compound 2,2-Dichloropropane in sample 04JAN10.D from x, y = 5.137, 0 to 5.279, 0; result = 2930                                                                                                               |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:19:49 AM | Manually integrate qualifier 97.0 of compound 2,2-Dichloropropane in sample 04JAN10.D from x, y = 5.151, 0 to 5.285, 0; result = 814                                                                                              |        |         | ✓       |           |

# Audit Trail report

| Name                              | User           | Time                 | Action                                                                                                                                  | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|-----------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:19:52 AM | Manually integrate qualifier41.0 of compound 2,2-Dichloropropane in sample 04JAN10.D from x, y = 5.151, 0 to 5.257, 0; result = 2246    |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:20:11 AM | Manually integrate qualifier65.0 of compound 1,1-Dichloroethane in sample 04JAN10.D from x, y = 4.323, 0 to 4.465, 0; result = 1347     |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:20:13 AM | Manually integrate qualifier83.0 of compound 1,1-Dichloroethane in sample 04JAN10.D from x, y = 4.342, 0 to 4.426, 0; result = 227      |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/5/2022 10:26:02 AM | Manually integrate compound cis-1,2-Dichloroethene in sample 04JAN10.D from x, y = 5.145, 0 to 5.282, 0; result = 2376                  |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:26:05 AM | Manually integrate qualifier61.0 of compound cis-1,2-Dichloroethene in sample 04JAN10.D from x, y = 5.151, 0 to 5.274, 0; result = 4139 |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:26:07 AM | Manually integrate qualifier98.0 of compound cis-1,2-Dichloroethene in sample 04JAN10.D from x, y = 5.176, 0 to 5.257, 0; result = 1525 |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:26:12 AM | Manually integrate qualifier72.0 of compound Methyl ethyl ketone in sample 04JAN10.D from x, y = 5.274, 0 to 5.343, 0; result = 435     |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/5/2022 10:26:18 AM | Manually integrate compound Bromochloromethane in sample 04JAN10.D from x, y = 5.463, 0 to 5.555, 0; result = 807                       |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:26:20 AM | Manually integrate qualifier49.0 of compound Bromochloromethane in sample 04JAN10.D from x, y = 5.472, 0 to 5.558, 0; result = 1686     |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:26:23 AM | Manually integrate qualifier85.0 of compound Chloroform in sample 04JAN10.D from x, y = 5.592, 0 to 5.734, 0; result = 2708             |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/5/2022 10:26:28 AM | Manually integrate compound Dibromofluoromethane in sample 04JAN10.D from x, y = 5.812, 0 to 5.915, 0; result = 2508                    |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:26:30 AM | Manually integrate qualifier191.5 of compound Dibromofluoromethane in sample 04JAN10.D from x, y = 5.809, 0 to 5.884, 0; result = 479   |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:26:37 AM | Manually integrate qualifier61.0 of compound 1,1,1-Trichloroethane in sample 04JAN10.D from x, y = 5.790, 0 to 5.890, 0; result = 1705  |        |         | ✓       |           |



# Audit Trail report

| Name                              | User           | Time                 | Action                                                                                                                                                                                                                      | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:26:42 AM | Manually integrate qualifier121.0 of compound Carbon tetrachloride in sample 04JAN10.D from x, y = 5.999, 0 to 6.068, 0; result = 903                                                                                       |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:26:46 AM | Manually integrate qualifier110.0 of compound 1,1-Dichloropropene in sample 04JAN10.D from x, y = 5.993, 0 to 6.074, 0; result = 1122                                                                                       |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:26:48 AM | Manually integrate qualifier77.0 of compound 1,1-Dichloropropene in sample 04JAN10.D from x, y = 6.013, 0 to 6.099, 0; result = 1052                                                                                        |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/5/2022 10:26:53 AM | Manually integrate compound 1,2-Dichloroethane-d4 in sample 04JAN10.D from x, y = 6.188, -35 to 6.283, 0; result = 1023                                                                                                     |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/5/2022 10:26:58 AM | Manually integrate compound 1,2-Dichloroethane-d4 in sample 04JAN10.D, from x, y = 6.197, 0 to 6.283, 0, result = 923; previous integration is from x, y = 6.188, -35 to 6.283, 0 and previous response = 1023.             |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:27:00 AM | Manually integrate qualifier65.0 of compound 1,2-Dichloroethane-d4 in sample 04JAN10.D from x, y = 6.199, 0 to 6.275, 0; result = 1927                                                                                      |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:27:34 AM | Manually integrate qualifier77.0 of compound Benzene in sample 04JAN10.D from x, y = 6.222, 0 to 6.339, 0; result = 1884                                                                                                    |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/5/2022 10:27:39 AM | Manually integrate compound 1,2-Dichloroethane in sample 04JAN10.D from x, y = 6.269, 0 to 6.386, 0; result = 2415                                                                                                          |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:27:41 AM | Manually integrate qualifier64.0 of compound 1,2-Dichloroethane in sample 04JAN10.D from x, y = 6.280, 0 to 6.378, 0; result = 761                                                                                          |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:27:43 AM | Manually integrate qualifier98.0 of compound 1,2-Dichloroethane in sample 04JAN10.D from x, y = 6.303, 0 to 6.386, 0; result = 119                                                                                          |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/5/2022 10:27:47 AM | Manually integrate compound Trichloroethene in sample 04JAN10.D from x, y = 6.989, 0 to 7.083, 0; result = 2372                                                                                                             |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:27:51 AM | Manually integrate qualifier 130.0 of compound Trichloroethene in sample 04JAN10.D, from x, y = 6.997, 0 to 7.072, 0, result = 2567; previous integration is from x, y = 6.997, 0 to 7.044, 0 and previous response = 2405. |        |         | ✓       |           |

# Audit Trail report

| Name                              | User           | Time                 | Action                                                                                                                                                                                                                                    | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:27:53 AM | Manually integrate qualifier97.0 of compound Trichloroethene in sample 04JAN10.D from x, y = 6.991, 0 to 7.078, 0; result = 1659                                                                                                          |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:27:59 AM | Manually integrate qualifier76.0 of compound 1,2-Dichloropropane in sample 04JAN10.D from x, y = 7.231, 0 to 7.321, 0; result = 733                                                                                                       |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/5/2022 10:28:03 AM | Manually integrate compound Dibromomethane in sample 04JAN10.D from x, y = 7.357, 0 to 7.424, 0; result = 902                                                                                                                             |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:28:06 AM | Manually integrate qualifier95.0 of compound Dibromomethane in sample 04JAN10.D from x, y = 7.357, 0 to 7.454, 0; result = 535                                                                                                            |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:28:09 AM | Manually integrate qualifier173.5 of compound Dibromomethane in sample 04JAN10.D from x, y = 7.360, 0 to 7.429, 0; result = 1002                                                                                                          |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:28:15 AM | Manually integrate qualifier85.0 of compound Bromodichloromethane in sample 04JAN10.D from x, y = 7.546, 0 to 7.633, 0; result = 1631                                                                                                     |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:28:17 AM | Manually integrate qualifier127.0 of compound Bromodichloromethane in sample 04JAN10.D from x, y = 7.569, 0 to 7.633, 0; result = 130                                                                                                     |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:28:23 AM | Manually integrate qualifier77.0 of compound cis-1,3-Dichloropropene in sample 04JAN10.D from x, y = 8.009, 0 to 8.107, 0; result = 922                                                                                                   |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:28:35 AM | Manually integrate qualifier39.0 of compound cis-1,3-Dichloropropene in sample 04JAN10.D from x, y = 8.037, 0 to 8.090, 0; result = 1459                                                                                                  |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:28:40 AM | Manually integrate qualifier99.0 of compound Toluene-d8 in sample 04JAN10.D from x, y = 8.271, 0 to 8.350, 0; result = 699                                                                                                                |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/5/2022 10:28:47 AM | Manually integrate compound trans-1,3-Dichloropropene in sample 04JAN10.D from x, y = 8.614, 0 to 8.684, 0; result = 1470                                                                                                                 |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:28:50 AM | Manually integrate qualifier 77.0 of compound trans-1,3-Dichloropropene in sample 04JAN10.D, from x, y = 8.601, 0 to 8.656, -10, result = 8023; previous integration is from x, y = 8.656, 57 to 8.709, 135 and previous response = 3575. |        |         | ✓       |           |

# Audit Trail report

| Name                              | User           | Time                 | Action                                                                                                                                                                                                                                                                     | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:29:03 AM | Manually integrate qualifier 77.0 of compound trans-1,3-Dichloropropene in sample 04JAN10.D, from x, y = 8.601, 0 to 8.656, 156, result = 6858; previous integration is from x, y = 8.601, 0 to 8.835, -10 and previous response = 8023.                                   |        |         | ✓       |           |
| CmdManuallyIntegrateDropBaseline  | BL2000\mchavez | 1/5/2022 10:29:04 AM | Drop baseline for qualifier 77.0 of compound trans-1,3-Dichloropropene in sample 04JAN10.D to y = 0, new integration is from x, y = 8.601, 0 to 8.835, 0 and new response = 7954; previous integration is from x, y = 8.601, 0 to 8.835, 156 and previous response = 6858. |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:29:09 AM | Manually integrate qualifier 77.0 of compound trans-1,3-Dichloropropene in sample 04JAN10.D, from x, y = 8.601, 0 to 8.648, 141, result = 368; previous integration is from x, y = 8.601, 0 to 8.835, 0 and previous response = 7954.                                      |        |         | ✓       |           |
| CmdManuallyIntegrateDropBaseline  | BL2000\mchavez | 1/5/2022 10:29:12 AM | Drop baseline for qualifier 77.0 of compound trans-1,3-Dichloropropene in sample 04JAN10.D to y = 0, new integration is from x, y = 8.601, 0 to 8.648, 0 and new response = 568; previous integration is from x, y = 8.601, 0 to 8.648, 141 and previous response = 368.   |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:29:19 AM | Manually integrate qualifier 39.0 of compound trans-1,3-Dichloropropene in sample 04JAN10.D from x, y = 8.614, 0 to 8.648, 26; result = 974                                                                                                                                |        |         | ✓       |           |
| CmdManuallyIntegrateDropBaseline  | BL2000\mchavez | 1/5/2022 10:29:21 AM | Drop baseline for qualifier 39.0 of compound trans-1,3-Dichloropropene in sample 04JAN10.D to y = 0, new integration is from x, y = 8.614, 0 to 8.648, 0 and new response = 1000; previous integration is from x, y = 8.614, 0 to 8.648, 26 and previous response = 974.   |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/5/2022 10:29:29 AM | Manually integrate compound 1,1,2-Trichloroethane in sample 04JAN10.D from x, y = 8.785, 0 to 8.843, 0; result = 960                                                                                                                                                       |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:29:31 AM | Manually integrate qualifier 97.0 of compound 1,1,2-Trichloroethane in sample 04JAN10.D from x, y = 8.782, 0 to 8.857, 0; result = 1099                                                                                                                                    |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:29:34 AM | Manually integrate qualifier 85.0 of compound 1,1,2-Trichloroethane in sample 04JAN10.D from x, y = 8.796, 0 to 8.851, 0; result = 418                                                                                                                                     |        |         | ✓       |           |

# Audit Trail report

| Name                              | User           | Time                 | Action                                                                                                                                                                                                                                 | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/5/2022 10:29:39 AM | Manually integrate compound Tetrachloroethene in sample 04JAN10.D from x, y = 8.899, 0 to 8.983, 0; result = 2105                                                                                                                      |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:29:43 AM | Manually integrate qualifier 165.8 of compound Tetrachloroethene in sample 04JAN10.D from x, y = 8.885, 0 to 9.019, 0; result = 2853                                                                                                   |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:29:48 AM | Manually integrate qualifier 78.0 of compound 1,3-Dichloropropane in sample 04JAN10.D from x, y = 8.952, 0 to 9.010, 0; result = 452                                                                                                   |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/5/2022 10:29:52 AM | Manually integrate compound Chlorodibromomethane in sample 04JAN10.D from x, y = 9.169, 0 to 9.256, 0; result = 1468                                                                                                                   |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:29:54 AM | Manually integrate qualifier 127.0 of compound Chlorodibromomethane in sample 04JAN10.D from x, y = 9.175, 0 to 9.242, 0; result = 1140                                                                                                |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/5/2022 10:29:58 AM | Manually integrate compound 1,2-Dibromoethane in sample 04JAN10.D from x, y = 9.278, 0 to 9.348, 0; result = 1299                                                                                                                      |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:30:00 AM | Manually integrate qualifier 109.0 of compound 1,2-Dibromoethane in sample 04JAN10.D from x, y = 9.275, 0 to 9.340, 0; result = 1039                                                                                                   |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:30:35 AM | Manually integrate qualifier 64.0 of compound Vinyl chloride in sample 04JAN15.D, from x, y = 1.476, 4348 to 1.540, 3059, result = 44384; previous integration is from x, y = 1.478, 954 to 1.687, 2147 and previous response = 61198. |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/5/2022 10:35:03 AM | Set SampleApproved = True for sample 04JAN15.D; previous value = False                                                                                                                                                                 |        |         | ✓       |           |
| CmdStartMethodEditing             | BL2000\mchavez | 1/5/2022 10:35:10 AM | Start method editing                                                                                                                                                                                                                   |        |         | ✓       |           |
| CmdImportMethodFromSample         | BL2000\mchavez | 1/5/2022 10:35:10 AM | Import method from sample 04JAN15.D                                                                                                                                                                                                    |        |         | ✓       |           |

# Audit Trail report

| Name                    | User           | Time                 | Action                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                              | Reason | Comment | Succeed | Exception |
|-------------------------|----------------|----------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdUpdateRetentionTimes | BL2000\mchavez | 1/5/2022 10:35:27 AM | Update retention time for compound 1,4-Dichlorobenzene; 1,3-Dichlorobenzene; 4-Chlorotoluene; 2-Chlorotoluene; 1,2,3-Trichloropropane; Bromobenzene; 1,1,2,2-Tetrachloroethane; p-Bromofluorobenzene; Bromoform; Styrene; o-Xylene; m+p-Xylenes; Ethylbenzene; 1,1,1,2-Tetrachloroethane; Chlorobenzene; 1,2-Dibromoethane; Chlorodibromomethane; 1,3-Dichloropropane; Tetrachloroethene; 1,1,2-Trichloroethane; trans-1,3-Dichloropropene; Toluene; Toluene-d8; cis-1,3-Dichloropropene; Bromodichloromethane; Dibromomethane; 1,2-Dichloropropane; Trichloroethene; 1,2-Dichloroethane; Benzene; 1,2-Dichloroethane-d4; 1,1-Dichloropropene; Carbon tetrachloride; 1,1,1-Trichloroethane; Dibromofluoromethane; Chloroform; Bromochloromethane; Methyl ethyl ketone; cis-1,2-Dichloroethene; 2,2-Dichloropropane; 1,1-Dichloroethane; Methyl tert-butyl ether (MTBE); trans-1,2-Dichloroethene; Methylene chloride; 1,1-Dichloroethene; Trichlorofluoromethane; Chloroethane; Bromomethane; Vinyl chloride; Chloromethane; Dichlorodifluoromethane; 1,4-Dichlorobenzene-d4; Chlorobenzene-d5; Fluorobenzene; 1,2-Dichlorobenzene; |        |         | ✓       |           |

# Audit Trail report

| Name                     | User           | Time                 | Action                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                               | Reason | Comment | Succeed | Exception |
|--------------------------|----------------|----------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdUpdateQualifierRatios | BL2000\mchavez | 1/5/2022 10:35:32 AM | Update qualifier ratios for compound 1,4-Dichlorobenzene; Update qualifier ratios for compound 1,3-Dichlorobenzene; Update qualifier ratios for compound 4-Chlorotoluene; Update qualifier ratios for compound 2-Chlorotoluene; Update qualifier ratios for compound 1,2,3-Trichloropropane; Update qualifier ratios for compound Bromobenzene; Update qualifier ratios for compound 1,1,2,2-Tetrachloroethane; Update qualifier ratios for compound p-Bromofluorobenzene; Update qualifier ratios for compound Bromoform; Update qualifier ratios for compound Styrene; Update qualifier ratios for compound o-Xylene; Update qualifier ratios for compound m+p-Xylenes; Update qualifier ratios for compound Ethylbenzene; Update qualifier ratios for compound 1,1,1,2-Tetrachloroethane; Update qualifier ratios for compound Chlorobenzene; Update qualifier ratios for compound 1,2-Dibromoethane; Update qualifier ratios for compound Chlorodibromomethane; Update qualifier ratios for compound 1,3-Dichloropropane; Update qualifier ratios for compound Tetrachloroethene; Update qualifier ratios for compound 1,1,2-Trichloroethane; Update qualifier ratios for compound trans-1,3-Dichloropropene; Update qualifier ratios for compound Toluene; Update qualifier ratios for compound Toluene-d8; Update qualifier ratios for compound cis-1,3-Dichloropropene; Update qualifier ratios for compound Bromodichloromethane; Update qualifier ratios for compound Dibromomethane; Update qualifier ratios for compound 1,2-Dichloropropane; Update qualifier ratios for compound Trichloroethene; Update qualifier ratios for compound 1,2-Dichloroethane; Update qualifier ratios for compound Benzene; Update qualifier ratios for compound 1,2-Dichloroethane-d4; Update qualifier ratios for compound 1,1-Dichloropropene; Update qualifier ratios for compound Carbon tetrachloride; Update qualifier ratios for compound 1,1,1-Trichloroethane; Update qualifier ratios for compound Dibromofluoromethane; Update |        |         | ✓       |           |

# Audit Trail report

| Name                              | User           | Time                 | Action                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                         | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
|                                   |                |                      | qualifier ratios for compound Chloroform; Update qualifier ratios for compound Bromochloromethane; Update qualifier ratios for compound Methyl ethyl ketone; Update qualifier ratios for compound cis-1,2-Dichloroethene; Update qualifier ratios for compound 2,2-Dichloropropane; Update qualifier ratios for compound 1,1-Dichloroethane; Update qualifier ratios for compound Methyl tert-butyl ether (MTBE); Update qualifier ratios for compound trans-1,2-Dichloroethene; Update qualifier ratios for compound Methylene chloride; Update qualifier ratios for compound 1,1-Dichloroethene; Update qualifier ratios for compound Trichlorofluoromethane; Update qualifier ratios for compound Chloroethane; Update qualifier ratios for compound Bromomethane; Update qualifier ratios for compound Vinyl chloride; Update qualifier ratios for compound Chloromethane; Update qualifier ratios for compound Dichlorodifluoromethane; Update qualifier ratios for compound 1,4-Dichlorobenzene-d4; Update qualifier ratios for compound Chlorobenzene-d5; Update qualifier ratios for compound Fluorobenzene; Update qualifier ratios for compound 1,2-Dichlorobenzene; |        |         |         |           |
| CmdApplyMethodToAllSamples        | BL2000\mchavez | 1/5/2022 10:35:43 AM | Apply method to all samples                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                    |        |         | ✓       |           |
| CmdMethodClear                    | BL2000\mchavez | 1/5/2022 10:35:43 AM | Clear method                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                   |        |         | ✓       |           |
| CmdEndMethodEditing               | BL2000\mchavez | 1/5/2022 10:35:43 AM | End method editing                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                             |        |         | ✓       |           |
| CmdQuantitate                     | BL2000\mchavez | 1/5/2022 10:36:02 AM | Quantitate all compounds in all samples                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                        |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/5/2022 10:37:04 AM | Manually integrate compound 2-Chlorotoluene in sample 04JAN10.D from x, y = 11.241, 0 to 11.353, 0; result = 1844                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                              |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/5/2022 10:37:15 AM | Manually integrate compound Bromobenzene in sample 04JAN10.D from x, y = 11.049, 0 to 11.127, 0; result = 2024                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                 |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:37:18 AM | Manually integrate qualifier 158.0 of compound Bromobenzene in sample 04JAN10.D from x, y = 11.063, 0 to 11.152, 0; result = 1934                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                              |        |         | ✓       |           |

# Audit Trail report

| Name                              | User           | Time                 | Action                                                                                                                                         | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/5/2022 10:37:23 AM | Manually integrate compound 1,1,2,2-Tetrachloroethane in sample 04JAN10.D from x, y = 11.085, 0 to 11.188, 0; result = 1142                    |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:37:25 AM | Manually integrate qualifier 85.0 of compound 1,1,2,2-Tetrachloroethane in sample 04JAN10.D from x, y = 11.071, 0 to 11.147, 0; result = 834   |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/5/2022 10:37:35 AM | Manually integrate compound Bromoform in sample 04JAN10.D from x, y = 10.597, 0 to 10.686, 0; result = 708                                     |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:37:36 AM | Manually integrate qualifier 174.5 of compound Bromoform in sample 04JAN10.D from x, y = 10.594, 0 to 10.698, 0; result = 258                  |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:37:38 AM | Manually integrate qualifier 170.5 of compound Bromoform in sample 04JAN10.D from x, y = 10.603, 0 to 10.672, 0; result = 339                  |        |         | ✓       |           |
| CmdSetLevelEnable                 | BL2000\mchavez | 1/5/2022 10:37:45 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound 1,1,2,2-Tetrachloroethane in sample 04JAN15.D; previous value = True |        |         | ✓       |           |
| CmdSetLevelEnable                 | BL2000\mchavez | 1/5/2022 10:37:53 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound 2-Chlorotoluene in sample 04JAN15.D; previous value = True           |        |         | ✓       |           |
| CmdSetLevelEnable                 | BL2000\mchavez | 1/5/2022 10:37:55 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound 4-Chlorotoluene in sample 04JAN15.D; previous value = True           |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:37:58 AM | Manually integrate qualifier 126.0 of compound 4-Chlorotoluene in sample 04JAN10.D from x, y = 11.367, 0 to 11.467, 0; result = 1839           |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:38:03 AM | Manually integrate qualifier 111.0 of compound 1,3-Dichlorobenzene in sample 04JAN10.D from x, y = 12.000, 0 to 12.061, 0; result = 1469       |        |         | ✓       |           |
| CmdSetLevelEnable                 | BL2000\mchavez | 1/5/2022 10:38:05 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound 1,3-Dichlorobenzene in sample 04JAN15.D; previous value = True       |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:38:13 AM | Manually integrate qualifier 111.0 of compound 1,2-Dichlorobenzene in sample 04JAN10.D from x, y = 12.432, 0 to 12.538, 0; result = 1190       |        |         | ✓       |           |
| CmdSetLevelEnable                 | BL2000\mchavez | 1/5/2022 10:38:15 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound 1,2-Dichlorobenzene in sample 04JAN15.D; previous value = True       |        |         | ✓       |           |



# Audit Trail report

| Name                              | User           | Time                 | Action                                                                                                                                                                                                                                                         | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdSetLevelEnable                 | BL2000\mchavez | 1/5/2022 10:38:19 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound 1,4-Dichlorobenzene in sample 04JAN15.D; previous value = True                                                                                                                       |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:38:25 AM | Manually integrate qualifier 148.0 of compound 1,2-Dichlorobenzene in sample 04JAN10.D from x, y = 12.468, 0 to 12.555, 0; result = 1894                                                                                                                       |        |         | ✓       |           |
| CmdSetLevelEnable                 | BL2000\mchavez | 1/5/2022 10:38:44 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound Styrene in sample 04JAN15.D; previous value = True                                                                                                                                   |        |         | ✓       |           |
| CmdSetLevelEnable                 | BL2000\mchavez | 1/5/2022 10:38:48 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound o-Xylene in sample 04JAN15.D; previous value = True                                                                                                                                  |        |         | ✓       |           |
| CmdSetLevelEnable                 | BL2000\mchavez | 1/5/2022 10:38:51 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound m+p-Xylenes in sample 04JAN15.D; previous value = True                                                                                                                               |        |         | ✓       |           |
| CmdSetLevelEnable                 | BL2000\mchavez | 1/5/2022 10:38:58 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound Ethylbenzene in sample 04JAN15.D; previous value = True                                                                                                                              |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:40:02 AM | Manually integrate qualifier 106.0 of compound Ethylbenzene in sample 04JAN10.D, from x, y = 9.883, 0 to 9.953, 0, result = 3266; previous integration is from x, y = 9.914, 0 to 9.953, 0 and previous response = 2097.                                       |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/5/2022 10:40:07 AM | Manually integrate compound 1,1,1,2-Tetrachloroethane in sample 04JAN10.D from x, y = 9.853, 0 to 9.939, 0; result = 1893                                                                                                                                      |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:40:11 AM | Manually integrate qualifier 133.0 of compound 1,1,1,2-Tetrachloroethane in sample 04JAN10.D from x, y = 9.841, 0 to 9.931, 0; result = 1911                                                                                                                   |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:40:23 AM | Manually integrate qualifier 114.0 of compound Chlorobenzene in sample 04JAN10.D from x, y = 9.783, 18 to 9.844, 0; result = 1827                                                                                                                              |        |         | ✓       |           |
| CmdManuallyIntegrateDropBaseline  | BL2000\mchavez | 1/5/2022 10:40:24 AM | Drop baseline for qualifier 114.0 of compound Chlorobenzene in sample 04JAN10.D to y = 0, new integration is from x, y = 9.783, 0 to 9.844, 0 and new response = 1861; previous integration is from x, y = 9.783, 18 to 9.844, 0 and previous response = 1827. |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/5/2022 10:41:20 AM | Set SampleApproved = True for sample 04JAN10.D; previous value = False                                                                                                                                                                                         |        |         | ✓       |           |

# Audit Trail report

| Name                              | User           | Time                 | Action                                                                                                                                                                                                                                                          | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:41:35 AM | Manually integrate qualifier 64.0 of compound Vinyl chloride in sample 04JAN11.D, from x, y = 1.487, 5730 to 1.520, 4652, result = 5622; previous integration is from x, y = 1.311, 0 to 1.679, 0 and previous response = 180129.                               |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:41:38 AM | Manually integrate qualifier 64.0 of compound Vinyl chloride in sample 04JAN11.D, from x, y = 1.484, 5832 to 1.520, 4652, result = 5972; previous integration is from x, y = 1.487, 5730 to 1.520, 4652 and previous response = 5622.                           |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:41:51 AM | Manually integrate qualifier 63.0 of compound 1,1-Dichloroethene in sample 04JAN11.D, from x, y = 2.663, 0 to 2.736, 0, result = 5268; previous integration is from x, y = 2.697, 0 to 2.736, 0 and previous response = 3135.                                   |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/5/2022 10:41:59 AM | Manually integrate compound trans-1,2-Dichloroethene in sample 04JAN11.D, from x, y = 3.678, 0 to 3.765, 0, result = 9821; previous integration is from x, y = 3.678, 0 to 3.718, 0 and previous response = 5041.                                               |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/5/2022 10:42:05 AM | Manually integrate compound Methyl tert-butyl ether (MTBE) in sample 04JAN11.D, from x, y = 3.687, 0 to 3.823, 182, result = 11769; previous integration is from x, y = 3.737, 0 to 3.804, 0 and previous response = 10323.                                     |        |         | ✓       |           |
| CmdManuallyIntegrateDropBaseline  | BL2000\mchavez | 1/5/2022 10:42:08 AM | Drop baseline for compound Methyl tert-butyl ether (MTBE) in sample 04JAN11.D to y = 0, new integration is from x, y = 3.687, 0 to 3.823, 0 and new response = 12515; previous integration is from x, y = 3.687, 0 to 3.823, 182 and previous response = 11769. |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:42:12 AM | Manually integrate qualifier 57.0 of compound Methyl tert-butyl ether (MTBE) in sample 04JAN11.D, from x, y = 3.681, 0 to 3.821, 0, result = 3045; previous integration is from x, y = 3.709, 0 to 3.776, 0 and previous response = 2643.                       |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:42:20 AM | Manually integrate qualifier 97.0 of compound 2,2-Dichloropropane in sample 04JAN11.D from x, y = 5.140, 0 to 5.240, 0; result = 3733                                                                                                                           |        |         | ✓       |           |

# Audit Trail report

| Name                              | User           | Time                 | Action                                                                                                                                                                                                                          | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:42:32 AM | Manually integrate qualifier 191.5 of compound Dibromofluoromethane in sample 04JAN11.D from x, y = 5.809, 0 to 5.918, 0; result = 2020                                                                                         |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:42:45 AM | Manually integrate qualifier 110.0 of compound 1,1-Dichloropropene in sample 04JAN11.D, from x, y = 5.985, 0 to 6.077, 0, result = 5349; previous integration is from x, y = 6.035, 0 to 6.077, 0 and previous response = 3323. |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:42:59 AM | Manually integrate qualifier 98.0 of compound 1,2-Dichloroethane in sample 04JAN11.D from x, y = 6.275, 0 to 6.381, 0; result = 648                                                                                             |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:43:02 AM | Manually integrate qualifier 64.0 of compound 1,2-Dichloroethane in sample 04JAN11.D, from x, y = 6.266, 0 to 6.361, 0, result = 3587; previous integration is from x, y = 6.317, 0 to 6.361, 0 and previous response = 2405.   |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:43:11 AM | Manually integrate qualifier 127.0 of compound Bromodichloromethane in sample 04JAN11.D from x, y = 7.549, 0 to 7.627, 0; result = 943                                                                                          |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/5/2022 10:43:21 AM | Manually integrate compound 1,1,2-Trichloroethane in sample 04JAN11.D, from x, y = 8.768, 0 to 8.882, 0, result = 5090; previous integration is from x, y = 8.818, 0 to 8.851, 0 and previous response = 2437.                  |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/5/2022 10:44:13 AM | Manually integrate compound 1,2,3-Trichloropropane in sample 04JAN11.D from x, y = 11.099, 0 to 11.174, 0; result = 1654                                                                                                        |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:44:16 AM | Manually integrate qualifier 112.0 of compound 1,2,3-Trichloropropane in sample 04JAN11.D from x, y = 11.096, 0 to 11.191, 0; result = 1059                                                                                     |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/5/2022 10:44:25 AM | Set SampleApproved = True for sample 04JAN11.D; previous value = False                                                                                                                                                          |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/5/2022 10:44:48 AM | Manually integrate compound 1,2,3-Trichloropropane in sample 04JAN12.D, from x, y = 11.099, 0 to 11.180, 0, result = 3200; previous integration is from x, y = 11.141, 0 to 11.180, 0 and previous response = 2198.             |        |         | ✓       |           |
| CmdSetLevelEnable                 | BL2000\mchavez | 1/5/2022 10:45:22 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound Chlorodibromomethane in sample 04JAN15.D; previous value = True                                                                                       |        |         | ✓       |           |

# Audit Trail report

| Name                               | User           | Time                 | Action                                                                                                                                                                                                                                                             | Reason | Comment | Succeed | Exception |
|------------------------------------|----------------|----------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdSetLevelEnable                  | BL2000\mchavez | 1/5/2022 10:45:30 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound Tetrachloroethene in sample 04JAN15.D; previous value = True                                                                                                                             |        |         | ✓       |           |
| CmdSetLevelEnable                  | BL2000\mchavez | 1/5/2022 10:45:37 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound 1,1,2-Trichloroethane in sample 04JAN15.D; previous value = True                                                                                                                         |        |         | ✓       |           |
| CmdSetLevelEnable                  | BL2000\mchavez | 1/5/2022 10:45:40 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound trans-1,3-Dichloropropene in sample 04JAN15.D; previous value = True                                                                                                                     |        |         | ✓       |           |
| CmdSetLevelEnable                  | BL2000\mchavez | 1/5/2022 10:45:45 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound Toluene in sample 04JAN15.D; previous value = True                                                                                                                                       |        |         | ✓       |           |
| CmdSetLevelEnable                  | BL2000\mchavez | 1/5/2022 10:45:57 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound cis-1,3-Dichloropropene in sample 04JAN15.D; previous value = True                                                                                                                       |        |         | ✓       |           |
| CmdManuallyIntegrate QualifierPeak | BL2000\mchavez | 1/5/2022 10:46:03 AM | Manually integrate qualifier 127.0 of compound Bromodichloromethane in sample 04JAN12.D from x, y = 7.541, 0 to 7.633, 0; result = 2111                                                                                                                            |        |         | ✓       |           |
| CmdManuallyIntegrate QualifierPeak | BL2000\mchavez | 1/5/2022 10:46:15 AM | Manually integrate qualifier 98.0 of compound 1,2-Dichloroethane in sample 04JAN12.D from x, y = 6.278, 83 to 6.370, 0; result = 1440                                                                                                                              |        |         | ✓       |           |
| CmdManuallyIntegrate DropBaseline  | BL2000\mchavez | 1/5/2022 10:46:16 AM | Drop baseline for qualifier 98.0 of compound 1,2-Dichloroethane in sample 04JAN12.D to y = 0, new integration is from x, y = 6.278, 0 to 6.370, 0 and new response = 1669; previous integration is from x, y = 6.278, 83 to 6.370, 0 and previous response = 1440. |        |         | ✓       |           |
| CmdManuallyIntegrate QualifierPeak | BL2000\mchavez | 1/5/2022 10:46:38 AM | Manually integrate qualifier 97.0 of compound 2,2-Dichloropropane in sample 04JAN12.D, from x, y = 5.143, 0 to 5.254, 0, result = 6975; previous integration is from x, y = 5.187, 0 to 5.229, 0 and previous response = 4210.                                     |        |         | ✓       |           |
| CmdManuallyIntegrate QualifierPeak | BL2000\mchavez | 1/5/2022 10:46:55 AM | Manually integrate qualifier 64.0 of compound Vinyl chloride in sample 04JAN12.D, from x, y = 1.473, 6379 to 1.526, 4265, result = 8175; previous integration is from x, y = 1.305, 0 to 1.676, 0 and previous response = 154800.                                  |        |         | ✓       |           |

# Audit Trail report

| Name                              | User           | Time                 | Action                                                                                                                                                                                                                                 | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:47:03 AM | Manually integrate qualifier 64.0 of compound Vinyl chloride in sample 04JAN12.D, from x, y = 1.467, 4922 to 1.529, 3954, result = 11779; previous integration is from x, y = 1.473, 6379 to 1.526, 4265 and previous response = 8175. |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/5/2022 10:47:11 AM | Set SampleApproved = True for sample 04JAN12.D; previous value = False                                                                                                                                                                 |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/5/2022 10:47:23 AM | Manually integrate qualifier 64.0 of compound Vinyl chloride in sample 04JAN13.D, from x, y = 1.470, 5496 to 1.517, 5210, result = 15113; previous integration is from x, y = 1.308, 0 to 1.679, 0 and previous response = 148305.     |        |         | ✓       |           |
| CmdSetLevelEnable                 | BL2000\mchavez | 1/5/2022 10:47:46 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound Chloroform in sample 04JAN15.D; previous value = True                                                                                                        |        |         | ✓       |           |
| CmdSetLevelEnable                 | BL2000\mchavez | 1/5/2022 10:47:57 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound 1,1-Dichloropropene in sample 04JAN15.D; previous value = True                                                                                               |        |         | ✓       |           |
| CmdSetLevelEnable                 | BL2000\mchavez | 1/5/2022 10:48:15 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound Trichloroethene in sample 04JAN15.D; previous value = True                                                                                                   |        |         | ✓       |           |
| CmdSetLevelEnable                 | BL2000\mchavez | 1/5/2022 10:48:21 AM | Set LevelEnable = False for calibration level 1, levelId = 20 of compound 1,2-Dichloropropane in sample 04JAN15.D; previous value = True                                                                                               |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/5/2022 10:48:59 AM | Set SampleApproved = True for sample 04JAN13.D; previous value = False                                                                                                                                                                 |        |         | ✓       |           |
| CmdQuantitate                     | BL2000\mchavez | 1/5/2022 10:49:20 AM | Quantitate all compounds in all samples                                                                                                                                                                                                |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/5/2022 10:53:33 AM | Set SampleApproved = True for sample 04JAN17.D; previous value = False                                                                                                                                                                 |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/5/2022 10:53:45 AM | Set SampleApproved = True for sample 04JAN19.D; previous value = False                                                                                                                                                                 |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/5/2022 10:53:56 AM | Set SampleApproved = True for sample 04JAN21.D; previous value = False                                                                                                                                                                 |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/5/2022 10:55:07 AM | Set SampleApproved = True for sample 04JAN23.D; previous value = False                                                                                                                                                                 |        |         | ✓       |           |

# Audit Trail report

| Name         | User           | Time                 | Action                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                       | Reason | Comment | Succeed | Exception |
|--------------|----------------|----------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdCalibrate | BL2000\mchavez | 1/5/2022 10:55:43 AM | Replace level QC with QC sample 04JAN23.D for compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, 1,2-Dichloroethane, Benzene, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1-Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Chloroethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, o-Xylene};<br>Replace level 8 with Calibration sample 04JAN21.D for compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, 1,2-Dichloroethane, Benzene, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1-Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl |        |         | ✓       |           |

# Audit Trail report

| Name | User | Time | Action                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                               | Reason | Comment | Succeed | Exception |
|------|------|------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
|      |      |      | ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Chloroethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, o-Xylene};<br>Replace level 7 with Calibration sample 04JAN19.D for compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, 1,2-Dichloroethane, Benzene, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1-Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Chloroethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, o-Xylene};<br>Replace level 6 with Calibration sample 04JAN17.D for compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, |        |         |         |           |

# Audit Trail report

| Name | User | Time | Action                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                      | Reason | Comment | Succeed | Exception |
|------|------|------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
|      |      |      | Bromodichloromethane,<br>Dibromomethane, 1,2-<br>Dichloropropane, Trichloroethene, 1,2-<br>Dichloroethane, Benzene, 1,2-<br>Dichloroethane-d4, 1,1-<br>Dichloropropene, Carbon tetrachloride,<br>Dibromofluoromethane, 1,1,1-<br>Trichloroethane, Chloroform,<br>Bromochloromethane, Methyl ethyl<br>ketone, cis-1,2-Dichloroethene, 2,2-<br>Dichloropropane, 1,1-Dichloroethane,<br>Methyl tert-butyl ether (MTBE), trans-<br>1,2-Dichloroethene, Methylene<br>chloride, 1,1-Dichloroethene,<br>Trichlorofluoromethane, Chloroethane,<br>Bromomethane, Vinyl chloride,<br>Chloromethane,<br>Dichlorodifluoromethane, o-Xylene};<br>Replace level 5 with Calibration sample<br>04JAN15.D for compounds {1,2-<br>Dichlorobenzene, 1,4-Dichlorobenzene,<br>1,3-Dichlorobenzene, 4-Chlorotoluene,<br>2-Chlorotoluene, 1,2,3-<br>Trichloropropane, 1,1,2,2-<br>Tetrachloroethane, Bromobenzene, p-<br>Bromofluorobenzene, Bromoform,<br>Styrene, m+p-Xylenes, Ethylbenzene,<br>1,1,1,2-Tetrachloroethane,<br>Chlorobenzene, 1,2-Dibromoethane,<br>Chlorodibromomethane, 1,3-<br>Dichloropropane, Tetrachloroethene,<br>1,1,2-Trichloroethane, trans-1,3-<br>Dichloropropene, Toluene, Toluene-d8,<br>cis-1,3-Dichloropropene,<br>Bromodichloromethane,<br>Dibromomethane, 1,2-<br>Dichloropropane, Trichloroethene, 1,2-<br>Dichloroethane, Benzene, 1,2-<br>Dichloroethane-d4, 1,1-<br>Dichloropropene, Carbon tetrachloride,<br>Dibromofluoromethane, 1,1,1-<br>Trichloroethane, Chloroform,<br>Bromochloromethane, Methyl ethyl<br>ketone, cis-1,2-Dichloroethene, 2,2-<br>Dichloropropane, 1,1-Dichloroethane,<br>Methyl tert-butyl ether (MTBE), trans-<br>1,2-Dichloroethene, Methylene<br>chloride, 1,1-Dichloroethene,<br>Trichlorofluoromethane, Chloroethane,<br>Bromomethane, Vinyl chloride,<br>Chloromethane,<br>Dichlorodifluoromethane, o-Xylene};<br>Replace level 4 with Calibration sample<br>04JAN13.D for compounds {1,2-<br>Dichlorobenzene, 1,4-Dichlorobenzene,<br>1,3-Dichlorobenzene, 4-Chlorotoluene,<br>2-Chlorotoluene, 1,2,3-<br>Trichloropropane, 1,1,2,2-<br>Tetrachloroethane, Bromobenzene, p- |        |         |         |           |



# Audit Trail report

| Name | User | Time | Action                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                         | Reason | Comment | Succeed | Exception |
|------|------|------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
|      |      |      | Bromofluorobenzene, Bromoform, Styrene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, 1,2-Dichloroethane, Benzene, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1-Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Chloroethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, o-Xylene};<br>Replace level 3 with Calibration sample 04JAN12.D for compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, 1,2-Dichloroethane, Benzene, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1-Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Chloroethane, Bromomethane, Vinyl chloride, |        |         |         |           |

# Audit Trail report

| Name | User | Time | Action                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                       | Reason | Comment | Succeed | Exception |
|------|------|------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
|      |      |      | Chloromethane,<br>Dichlorodifluoromethane, o-Xylene};<br>Replace level 2 with Calibration sample<br>04JAN11.D for compounds {1,2-<br>Dichlorobenzene, 1,4-Dichlorobenzene,<br>1,3-Dichlorobenzene, 4-Chlorotoluene,<br>2-Chlorotoluene, 1,2,3-<br>Trichloropropane, 1,1,2,2-<br>Tetrachloroethane, Bromobenzene, p-<br>Bromofluorobenzene, Bromoform,<br>Styrene, m+p-Xylenes, Ethylbenzene,<br>1,1,1,2-Tetrachloroethane,<br>Chlorobenzene, 1,2-Dibromoethane,<br>Chlorodibromomethane, 1,3-<br>Dichloropropane, Tetrachloroethene,<br>1,1,2-Trichloroethane, trans-1,3-<br>Dichloropropene, Toluene, Toluene-d8,<br>cis-1,3-Dichloropropene,<br>Bromodichloromethane,<br>Dibromomethane, 1,2-<br>Dichloropropane, Trichloroethene, 1,2-<br>Dichloroethane, Benzene, 1,2-<br>Dichloroethane-d4, 1,1-<br>Dichloropropene, Carbon tetrachloride,<br>Dibromofluoromethane, 1,1,1-<br>Trichloroethane, Chloroform,<br>Bromochloromethane, Methyl ethyl<br>ketone, cis-1,2-Dichloroethene, 2,2-<br>Dichloropropane, 1,1-Dichloroethane,<br>Methyl tert-butyl ether (MTBE), trans-<br>1,2-Dichloroethene, Methylene<br>chloride, 1,1-Dichloroethene,<br>Trichlorofluoromethane, Chloroethane,<br>Bromomethane, Vinyl chloride,<br>Chloromethane,<br>Dichlorodifluoromethane, o-Xylene};<br>Replace level 1 with Calibration sample<br>04JAN10.D for compounds {1,2-<br>Dichlorobenzene, 1,4-Dichlorobenzene,<br>1,3-Dichlorobenzene, 4-Chlorotoluene,<br>2-Chlorotoluene, 1,2,3-<br>Trichloropropane, 1,1,2,2-<br>Tetrachloroethane, Bromobenzene, p-<br>Bromofluorobenzene, Bromoform,<br>Styrene, m+p-Xylenes, Ethylbenzene,<br>1,1,1,2-Tetrachloroethane,<br>Chlorobenzene, 1,2-Dibromoethane,<br>Chlorodibromomethane, 1,3-<br>Dichloropropane, Tetrachloroethene,<br>1,1,2-Trichloroethane, trans-1,3-<br>Dichloropropene, Toluene, Toluene-d8,<br>cis-1,3-Dichloropropene,<br>Bromodichloromethane,<br>Dibromomethane, 1,2-<br>Dichloropropane, Trichloroethene, 1,2-<br>Dichloroethane, Benzene, 1,2-<br>Dichloroethane-d4, 1,1-<br>Dichloropropene, Carbon tetrachloride,<br>Dibromofluoromethane, 1,1,1- |        |         |         |           |

# Audit Trail report

| Name                                | User           | Time                 | Action                                                                                                                                                                                                                                                                                                                                                          | Reason | Comment | Succeed | Exception |
|-------------------------------------|----------------|----------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
|                                     |                |                      | Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Chloroethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, o-Xylene}; |        |         |         |           |
| CmdQuantitate                       | BL2000\mchavez | 1/5/2022 10:55:58 AM | Quantitate all compounds in all samples                                                                                                                                                                                                                                                                                                                         |        |         | ✓       |           |
| CmdManuallyIntegratePeak            | BL2000\mchavez | 1/5/2022 11:01:11 AM | Manually integrate compound Methylene chloride in sample 04JAN09.D from x, y = 3.296, 0 to 3.383, 0; result = 1661                                                                                                                                                                                                                                              |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak   | BL2000\mchavez | 1/5/2022 11:01:17 AM | Manually integrate qualifier 84.0 of compound Methylene chloride in sample 04JAN09.D from x, y = 3.299, 0 to 3.369, 0; result = 1075                                                                                                                                                                                                                            |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak   | BL2000\mchavez | 1/5/2022 11:01:19 AM | Manually integrate qualifier 86.0 of compound Methylene chloride in sample 04JAN09.D from x, y = 3.294, 0 to 3.413, 0; result = 694                                                                                                                                                                                                                             |        |         | ✓       |           |
| CmdManuallyIntegratePeak            | BL2000\mchavez | 1/5/2022 11:02:10 AM | Manually integrate compound Vinyl chloride in sample 04JAN09.D from x, y = 1.467, 0 to 1.520, 0; result = 73                                                                                                                                                                                                                                                    |        |         | ✓       |           |
| CmdStartMethodEditing               | BL2000\mchavez | 1/5/2022 11:02:39 AM | Start method editing                                                                                                                                                                                                                                                                                                                                            |        |         | ✓       |           |
| CmdImportMethodFromSample           | BL2000\mchavez | 1/5/2022 11:02:39 AM | Import method from sample 04JAN09.D                                                                                                                                                                                                                                                                                                                             |        |         | ✓       |           |
| CmdSetMethodTargetCompoundAttribute | BL2000\mchavez | 1/5/2022 11:03:13 AM | Set CurveFit = fitAverageOfResponseFactors for compound Bromomethane; previous value = fitQuadratic                                                                                                                                                                                                                                                             |        |         | ✓       |           |
| CmdSetMethodTargetCompoundAttribute | BL2000\mchavez | 1/5/2022 11:03:16 AM | Set CurveFitWeight = weightEqual for compound Bromomethane; previous value = weightOneOverX                                                                                                                                                                                                                                                                     |        |         | ✓       |           |
| CmdApplyMethodToAllSamples          | BL2000\mchavez | 1/5/2022 11:03:28 AM | Apply method to all samples                                                                                                                                                                                                                                                                                                                                     |        |         | ✓       |           |
| CmdMethodClear                      | BL2000\mchavez | 1/5/2022 11:03:28 AM | Clear method                                                                                                                                                                                                                                                                                                                                                    |        |         | ✓       |           |
| CmdEndMethodEditing                 | BL2000\mchavez | 1/5/2022 11:03:29 AM | End method editing                                                                                                                                                                                                                                                                                                                                              |        |         | ✓       |           |
| CmdQuantitate                       | BL2000\mchavez | 1/5/2022 11:03:49 AM | Quantitate all compounds in all samples                                                                                                                                                                                                                                                                                                                         |        |         | ✓       |           |
| CmdManuallyIntegratePeak            | BL2000\mchavez | 1/5/2022 11:05:06 AM | Manually integrate compound Chloroethane in sample 04JAN12.D, from x, y = 1.863, 1400 to 1.922, 1881, result = 14646; previous integration is from x, y = 1.863, 1400 to 1.958, 1400 and previous response = 16843.                                                                                                                                             |        |         | ✓       |           |

# Audit Trail report

| Name                     | User           | Time                 | Action                                                                                                                                                                                                            | Reason | Comment | Succeed | Exception |
|--------------------------|----------------|----------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/5/2022 11:05:19 AM | Manually integrate compound Chloroethane in sample 04JAN11.D, from x, y = 1.869, 1143 to 1.930, 1702, result = 8052; previous integration is from x, y = 1.869, 1143 to 1.941, 1143 and previous response = 9540. |        |         | ✓       |           |

# Audit Trail report

| Name         | User           | Time                 | Action                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                 | Reason | Comment | Succeed | Exception |
|--------------|----------------|----------------------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdCalibrate | BL2000\mchavez | 1/5/2022 11:05:53 AM | Replace level QC with QC sample 04JAN23.D for compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, o-Xylene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, 1,2-Dichloroethane, Benzene, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1-Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, Chloroethane}; Replace level 8 with Calibration sample 04JAN21.D for compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, o-Xylene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, 1,2-Dichloroethane, Benzene, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1- |        |         | ✓       |           |

# Audit Trail report

| Name | User | Time | Action                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                    | Reason | Comment | Succeed | Exception |
|------|------|------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
|      |      |      | Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, Chloroethane}; Replace level 7 with Calibration sample 04JAN19.D for compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, o-Xylene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, 1,2-Dichloroethane, Benzene, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1-Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, Chloroethane}; Replace level 6 with Calibration sample 04JAN17.D for compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, o-Xylene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3- |        |         |         |           |

# Audit Trail report

| Name | User | Time | Action                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           | Reason | Comment | Succeed | Exception |
|------|------|------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
|      |      |      | Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, 1,2-Dichloroethane, Benzene, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1-Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, Chloroethane}; Replace level 5 with Calibration sample 04JAN15.D for compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, o-Xylene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, 1,2-Dichloroethane, Benzene, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1-Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, Chloroethane}; Replace level 4 with Calibration sample 04JAN13.D for |        |         |         |           |

# Audit Trail report

| Name | User | Time | Action                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                | Reason | Comment | Succeed | Exception |
|------|------|------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
|      |      |      | compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, o-Xylene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, 1,2-Dichloroethane, Benzene, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1-Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, Chloroethane}; Replace level 3 with Calibration sample 04JAN12.D for compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, o-Xylene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, 1,2-Dichloroethane, Benzene, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1-Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl |        |         |         |           |



# Audit Trail report

| Name | User | Time | Action                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           | Reason | Comment | Succeed | Exception |
|------|------|------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
|      |      |      | ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, Chloroethane}; Replace level 2 with Calibration sample 04JAN11.D for compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, o-Xylene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, 1,2-Dichloroethane, Benzene, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1-Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, Chloroethane}; Replace level 1 with Calibration sample 04JAN10.D for compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, o-Xylene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3- |        |         |         |           |

# Audit Trail report

| Name              | User           | Time                 | Action                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                      | Reason | Comment | Succeed | Exception |
|-------------------|----------------|----------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
|                   |                |                      | Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, 1,2-Dichloroethane, Benzene, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1-Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, Chloroethane}; |        |         |         |           |
| CmdQuantitate     | BL2000\mchavez | 1/5/2022 11:06:12 AM | Quantitate all compounds in all samples                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                     |        |         | ✓       |           |
| CmdQuantitate     | BL2000\mchavez | 1/5/2022 11:07:28 AM | Quantitate all compounds in all samples                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                     |        |         | ✓       |           |
| CmdSaveBatchTable | BL2000\mchavez | 1/5/2022 11:07:47 AM | Save batch<br>D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           |        |         | ✓       |           |
| CmdOpenBatchTable | BL2000\mchavez | 1/9/2022 8:45:32 PM  | Open batch<br>D:\Org\Data\VOA5975C\VG010422\VG010422_8260B.batch.bin                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                        |        |         | ✓       |           |
| CmdSetLevelEnable | BL2000\mchavez | 1/9/2022 8:47:42 PM  | Set LevelEnable = True for calibration level 1, levelId = 30 of compound o-Xylene in sample 04JAN09.D; previous value = False                                                                                                                                                                                                                                                                                                                                                                                                                                                                                               |        |         | ✓       |           |
| CmdQuantitate     | BL2000\mchavez | 1/9/2022 8:48:01 PM  | Quantitate all compounds in all samples                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                     |        |         | ✓       |           |
| CmdSetLevelEnable | BL2000\mchavez | 1/9/2022 8:48:47 PM  | Set LevelEnable = True for calibration level 1, levelId = 30 of compound m+p-Xylenes in sample 04JAN09.D; previous value = False                                                                                                                                                                                                                                                                                                                                                                                                                                                                                            |        |         | ✓       |           |
| CmdQuantitate     | BL2000\mchavez | 1/9/2022 8:49:03 PM  | Quantitate all compounds in all samples                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                     |        |         | ✓       |           |
| CmdSetLevelEnable | BL2000\mchavez | 1/9/2022 8:49:35 PM  | Set LevelEnable = True for calibration level 1, levelId = 30 of compound Ethylbenzene in sample 04JAN09.D; previous value = False                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           |        |         | ✓       |           |
| CmdQuantitate     | BL2000\mchavez | 1/9/2022 8:49:50 PM  | Quantitate all compounds in all samples                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                     |        |         | ✓       |           |
| CmdSetLevelEnable | BL2000\mchavez | 1/9/2022 8:50:18 PM  | Set LevelEnable = True for calibration level 1, levelId = 30 of compound Styrene in sample 04JAN09.D; previous value = False                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                |        |         | ✓       |           |

# Audit Trail report

| Name              | User           | Time                | Action                                                                                                                                         | Reason | Comment | Succeed | Exception |
|-------------------|----------------|---------------------|------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdQuantitate     | BL2000\mchavez | 1/9/2022 8:50:35 PM | Quantitate all compounds in all samples                                                                                                        |        |         | ✓       |           |
| CmdSetLevelEnable | BL2000\mchavez | 1/9/2022 8:50:51 PM | Set LevelEnable = True for calibration level 1, levelId = 30 of compound Tetrachloroethene in sample 04JAN09.D; previous value = False         |        |         | ✓       |           |
| CmdQuantitate     | BL2000\mchavez | 1/9/2022 8:51:06 PM | Quantitate all compounds in all samples                                                                                                        |        |         | ✓       |           |
| CmdSetLevelEnable | BL2000\mchavez | 1/9/2022 8:51:27 PM | Set LevelEnable = True for calibration level 1, levelId = 30 of compound Toluene in sample 04JAN09.D; previous value = False                   |        |         | ✓       |           |
| CmdQuantitate     | BL2000\mchavez | 1/9/2022 8:51:42 PM | Quantitate all compounds in all samples                                                                                                        |        |         | ✓       |           |
| CmdSetLevelEnable | BL2000\mchavez | 1/9/2022 8:52:26 PM | Set LevelEnable = True for calibration level 1, levelId = 30 of compound trans-1,3-Dichloropropene in sample 04JAN09.D; previous value = False |        |         | ✓       |           |
| CmdQuantitate     | BL2000\mchavez | 1/9/2022 8:52:42 PM | Quantitate all compounds in all samples                                                                                                        |        |         | ✓       |           |
| CmdSetLevelEnable | BL2000\mchavez | 1/9/2022 8:52:55 PM | Set LevelEnable = False for calibration level 1, levelId = 30 of compound trans-1,3-Dichloropropene in sample 04JAN09.D; previous value = True |        |         | ✓       |           |
| CmdSetLevelEnable | BL2000\mchavez | 1/9/2022 8:53:25 PM | Set LevelEnable = True for calibration level 1, levelId = 30 of compound Benzene in sample 04JAN09.D; previous value = False                   |        |         | ✓       |           |
| CmdQuantitate     | BL2000\mchavez | 1/9/2022 8:53:41 PM | Quantitate all compounds in all samples                                                                                                        |        |         | ✓       |           |
| CmdSetLevelEnable | BL2000\mchavez | 1/9/2022 8:54:07 PM | Set LevelEnable = True for calibration level 1, levelId = 30 of compound Chloroform in sample 04JAN09.D; previous value = False                |        |         | ✓       |           |
| CmdQuantitate     | BL2000\mchavez | 1/9/2022 8:54:23 PM | Quantitate all compounds in all samples                                                                                                        |        |         | ✓       |           |
| CmdSetLevelEnable | BL2000\mchavez | 1/9/2022 8:54:39 PM | Set LevelEnable = True for calibration level 1, levelId = 30 of compound 1,3-Dichlorobenzene in sample 04JAN09.D; previous value = False       |        |         | ✓       |           |
| CmdSetLevelEnable | BL2000\mchavez | 1/9/2022 8:54:49 PM | Set LevelEnable = True for calibration level 1, levelId = 30 of compound 1,4-Dichlorobenzene in sample 04JAN09.D; previous value = False       |        |         | ✓       |           |
| CmdSetLevelEnable | BL2000\mchavez | 1/9/2022 8:54:54 PM | Set LevelEnable = True for calibration level 1, levelId = 30 of compound 1,2-Dichlorobenzene in sample 04JAN09.D; previous value = False       |        |         | ✓       |           |
| CmdQuantitate     | BL2000\mchavez | 1/9/2022 8:55:10 PM | Quantitate all compounds in all samples                                                                                                        |        |         | ✓       |           |

# Audit Trail report

| Name                         | User           | Time                | Action                                                                                                                                  | Reason | Comment | Succeed | Exception |
|------------------------------|----------------|---------------------|-----------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdSetLevelEnable            | BL2000\mchavez | 1/9/2022 8:56:06 PM | Set LevelEnable = True for calibration level 1, levelId = 30 of compound 1,2-Dichloroethane in sample 04JAN09.D; previous value = False |        |         | ✓       |           |
| CmdQuantitate                | BL2000\mchavez | 1/9/2022 8:56:22 PM | Quantitate all compounds in all samples                                                                                                 |        |         | ✓       |           |
| CmdImportSamplesFromWorklist | BL2000\mchavez | 1/9/2022 8:56:50 PM | Add samples from worklist: D:\Org\Data\VOA5975C\VG010422\04JAN15CC.D                                                                    |        |         | ✓       |           |
| CmdSetSampleAttribute        | BL2000\mchavez | 1/9/2022 8:57:23 PM | Set SampleType = Calibration for sample 04JAN15CC.D; previous value = Sample                                                            |        |         | ✓       |           |
| CmdSetSampleAttribute        | BL2000\mchavez | 1/9/2022 8:57:29 PM | Set LevelName = 5 for sample 04JAN15CC.D; previous value =                                                                              |        |         | ✓       |           |
| CmdQuantitate                | BL2000\mchavez | 1/9/2022 8:57:56 PM | Quantitate all compounds in all samples                                                                                                 |        |         | ✓       |           |
| CmdSetSampleAttribute        | BL2000\mchavez | 1/9/2022 8:58:36 PM | Set SampleType = CC for sample 04JAN15CC.D; previous value = Calibration                                                                |        |         | ✓       |           |
| CmdSetSampleAttribute        | BL2000\mchavez | 1/9/2022 8:58:43 PM | Set LevelName = CC for sample 04JAN15CC.D; previous value = 5                                                                           |        |         | ✓       |           |
| CmdSetSampleAttribute        | BL2000\mchavez | 1/9/2022 8:59:05 PM | Set UserDefined = Reimported midpoint as CC for sample 04JAN15CC.D; previous value =                                                    |        |         | ✓       |           |
| CmdSetSampleAttribute        | BL2000\mchavez | 1/9/2022 8:59:31 PM | Set SampleName = CC010422 for sample 04JAN15CC.D; previous value = ICAL010422_5                                                         |        |         | ✓       |           |

# Audit Trail report

| Name                       | User           | Time                | Action                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                              | Reason | Comment | Succeed | Exception |
|----------------------------|----------------|---------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdCalibrate               | BL2000\mchavez | 1/9/2022 8:59:53 PM | Replace level CC with CC sample 04JAN15CC.D for compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, o-Xylene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, Benzene, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1-Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Chloroethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, 1,2-Dichloroethane}; |        |         | ✓       |           |
| CmdQuantitate              | BL2000\mchavez | 1/9/2022 9:00:09 PM | Quantitate all compounds in all samples                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                             |        |         | ✓       |           |
| CmdStartMethodEditing      | BL2000\mchavez | 1/9/2022 9:00:22 PM | Start method editing                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                |        |         | ✓       |           |
| CmdImportMethodFrom Sample | BL2000\mchavez | 1/9/2022 9:00:22 PM | Import method from sample 04JAN23.D                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                 |        |         | ✓       |           |
| CmdSaveMethodAs            | BL2000\mchavez | 1/9/2022 9:00:57 PM | Save method to file \\MASSHUNTER\Org\Data\Methods\Quant\VOA5975C\VOA5975C_010422_CAL.m                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                              |        |         | ✓       |           |
| CmdSaveMethodAs            | BL2000\mchavez | 1/9/2022 9:02:42 PM | Save method to file \\MASSHUNTER\Org\Data\Methods\Quant\VOA5975C\VOA5975C_010422_CAL\VOA5975C_8260B_SHT_DoD_L4_010422.m                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                             |        |         | ✓       |           |
| CmdMethodClear             | BL2000\mchavez | 1/9/2022 9:02:55 PM | Clear method                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                        |        |         | ✓       |           |
| CmdEndMethodEditing        | BL2000\mchavez | 1/9/2022 9:02:56 PM | End method editing                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                  |        |         | ✓       |           |
| CmdStartMethodEditing      | BL2000\mchavez | 1/9/2022 9:03:07 PM | Start method editing                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                |        |         | ✓       |           |

# Audit Trail report

| Name                              | User           | Time                 | Action                                                                                                                      | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|-----------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdImportMethodFromFile           | BL2000\mchavez | 1/9/2022 9:03:07 PM  | Import method from file \\MASSHUNTER\Org\Data\Methods\Quant\VOA5975C\VOA5975C_010422_CAL\VOA5975C_8260B_SHT_DoD_L4_010422.m |        |         | ✓       |           |
| CmdApplyMethodToAllSamples        | BL2000\mchavez | 1/9/2022 9:03:19 PM  | Apply method to all samples                                                                                                 |        |         | ✓       |           |
| CmdMethodClear                    | BL2000\mchavez | 1/9/2022 9:03:19 PM  | Clear method                                                                                                                |        |         | ✓       |           |
| CmdEndMethodEditing               | BL2000\mchavez | 1/9/2022 9:03:20 PM  | End method editing                                                                                                          |        |         | ✓       |           |
| CmdQuantitate                     | BL2000\mchavez | 1/9/2022 9:03:36 PM  | Quantitate all compounds in all samples                                                                                     |        |         | ✓       |           |
| CmdSaveBatchTable                 | BL2000\mchavez | 1/9/2022 9:04:21 PM  | Save batch D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin                                              |        |         | ✓       |           |
| CmdOpenBatchTable                 | BL2000\mchavez | 1/10/2022 2:13:24 PM | Open batch D:\Org\Data\VOA5975C\VG010422\VG010422_8260B.batch.bin                                                           |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/10/2022 2:13:38 PM | Set SampleApproved = True for sample 04JAN08.D; previous value = False                                                      |        |         | ✓       |           |
| CmdZeroOutPeak                    | BL2000\mchavez | 1/10/2022 2:14:50 PM | Zero out primary peak of compound Chloromethane in sample 04JAN09.D                                                         |        |         | ✓       |           |
| CmdZeroOutPeak                    | BL2000\mchavez | 1/10/2022 2:14:56 PM | Zero out primary peak of compound Vinyl chloride in sample 04JAN09.D                                                        |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/10/2022 2:15:19 PM | Manually integrate compound Benzene in sample 04JAN09.D from x, y = 6.250, 0 to 6.311, 0; result = 381                      |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 2:15:21 PM | Manually integrate qualifier 77.0 of compound Benzene in sample 04JAN09.D from x, y = 6.258, 0 to 6.308, 0; result = 86     |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/10/2022 2:16:46 PM | Set SampleApproved = True for sample 04JAN09.D; previous value = False                                                      |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/10/2022 2:17:02 PM | Set UserAnnotation = NI for compound Methylene chloride in sample 04JAN09.D; previous value =                               |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/10/2022 2:17:09 PM | Set UserAnnotation = NI for compound Benzene in sample 04JAN09.D; previous value =                                          |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/10/2022 2:18:45 PM | Set UserAnnotation = NI for compound Tetrachloroethene in sample 04JAN10.D; previous value =                                |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/10/2022 2:18:48 PM | Set UserAnnotation = NI for compound Chlorodibromomethane in sample 04JAN10.D; previous value =                             |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/10/2022 2:18:53 PM | Set UserAnnotation = NI for compound 1,2-Dibromoethane in sample 04JAN10.D; previous value =                                |        |         | ✓       |           |

# Audit Trail report

| Name                              | User           | Time                 | Action                                                                                                                                                                                                                              | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/10/2022 2:18:58 PM | Set UserAnnotation = NI for compound 1,1,1,2-Tetrachloroethane in sample 04JAN10.D; previous value =                                                                                                                                |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/10/2022 2:19:02 PM | Set UserAnnotation = NI for compound Bromoform in sample 04JAN10.D; previous value =                                                                                                                                                |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/10/2022 2:19:08 PM | Set UserAnnotation = NI for compound 1,1,2,2-Tetrachloroethane in sample 04JAN10.D; previous value =                                                                                                                                |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/10/2022 2:19:13 PM | Set UserAnnotation = NI for compound Bromobenzene in sample 04JAN10.D; previous value =                                                                                                                                             |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/10/2022 2:19:30 PM | Set UserAnnotation = NI for compound 2-Chlorotoluene in sample 04JAN10.D; previous value =                                                                                                                                          |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/10/2022 2:20:15 PM | Set UserAnnotation = GT for compound Chloroethane in sample 04JAN11.D; previous value =                                                                                                                                             |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/10/2022 2:20:34 PM | Set UserAnnotation = LT for compound trans-1,2-Dichloroethene in sample 04JAN11.D; previous value =                                                                                                                                 |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/10/2022 2:25:39 PM | Set UserAnnotation = LT for compound Methyl tert-butyl ether (MTBE) in sample 04JAN11.D; previous value =                                                                                                                           |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/10/2022 2:26:14 PM | Set UserAnnotation = LT for compound 1,1,2-Trichloroethane in sample 04JAN11.D; previous value =                                                                                                                                    |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/10/2022 2:26:26 PM | Set UserAnnotation = NI for compound 1,2,3-Trichloropropane in sample 04JAN11.D; previous value =                                                                                                                                   |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/10/2022 2:26:46 PM | Set UserAnnotation = LT for compound 1,2,3-Trichloropropane in sample 04JAN12.D; previous value =                                                                                                                                   |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/10/2022 2:26:59 PM | Set UserAnnotation = GT for compound Chloroethane in sample 04JAN12.D; previous value =                                                                                                                                             |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 3:00:42 PM | Manually integrate qualifier 148.0 of compound 1,4-Dichlorobenzene in sample 04JAN10.D, from x, y = 12.109, 0 to 12.145, 0, result = 2520; previous integration is from x, y = 12.084, 0 to 12.145, 0 and previous response = 3603. |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 3:00:52 PM | Manually integrate qualifier 111.0 of compound 1,4-Dichlorobenzene in sample 04JAN10.D, from x, y = 12.123, 0 to 12.148, 0, result = 1067; previous integration is from x, y = 12.075, 0 to 12.123, 0 and previous response = 3515. |        |         | ✓       |           |

# Audit Trail report

| Name                              | User           | Time                 | Action                                                                                                                                                                                                                  | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/10/2022 3:01:20 PM | Manually integrate qualifier 91.0 of compound o-Xylene in sample 04JAN10.D, from x, y = 10.405, 0 to 10.483, 0, result = 6062; previous integration is from x, y = 10.405, 0 to 10.466, 0 and previous response = 6034. |        |         | ✓       |           |
| CmdClearManualIntegration         | BL2000\mchavez | 1/10/2022 3:01:29 PM | Clear manual integration of qualifier 91.0 for compound o-Xylene in sample 04JAN10.D                                                                                                                                    |        |         | ✓       |           |
| CmdSetLevelEnable                 | BL2000\mchavez | 1/10/2022 3:07:00 PM | Set LevelEnable = False for calibration level 1, levelId = 30 of compound o-Xylene in sample 04JAN23.D; previous value = True                                                                                           |        |         | ✓       |           |
| CmdQuantitate                     | BL2000\mchavez | 1/10/2022 3:07:39 PM | Quantitate all compounds in all samples                                                                                                                                                                                 |        |         | ✓       |           |
| CmdSaveBatchTable                 | BL2000\mchavez | 1/10/2022 3:12:09 PM | Save batch<br>D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin                                                                                                                                       |        |         | ✓       |           |
| CmdOpenBatchTable                 | BL2000\mchavez | 1/11/2022 8:47:03 AM | Open batch<br>D:\Org\Data\VOA5975C\VG010422\VG010422_8260B.batch.bin                                                                                                                                                    |        |         | ✓       |           |
| CmdStartMethodEditing             | BL2000\mchavez | 1/11/2022 8:47:16 AM | Start method editing                                                                                                                                                                                                    |        |         | ✓       |           |
| CmdImportMethodFromSample         | BL2000\mchavez | 1/11/2022 8:47:16 AM | Import method from sample 04JAN01.D                                                                                                                                                                                     |        |         | ✓       |           |
| CmdSaveMethodAs                   | BL2000\mchavez | 1/11/2022 8:47:26 AM | Save method to file<br>\\MASSHUNTER\Org\Data\Methods\Quant\VOA5975C\VOA5975C_010422_CAL\VOA5975C_8260B_SHT_DoD_L4_010422.m                                                                                              |        |         | ✓       |           |
| CmdApplyMethodToAllSamples        | BL2000\mchavez | 1/11/2022 8:48:57 AM | Apply method to all samples                                                                                                                                                                                             |        |         | ✓       |           |
| CmdMethodClear                    | BL2000\mchavez | 1/11/2022 8:48:57 AM | Clear method                                                                                                                                                                                                            |        |         | ✓       |           |
| CmdEndMethodEditing               | BL2000\mchavez | 1/11/2022 8:48:58 AM | End method editing                                                                                                                                                                                                      |        |         | ✓       |           |
| CmdQuantitate                     | BL2000\mchavez | 1/11/2022 8:49:22 AM | Quantitate all compounds in all samples                                                                                                                                                                                 |        |         | ✓       |           |
| CmdSaveBatchTable                 | BL2000\mchavez | 1/11/2022 8:54:59 AM | Save batch<br>D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin                                                                                                                                       |        |         | ✓       |           |
| CmdOpenBatchTable                 | BL2000\mchavez | 2/28/2022 1:48:49 PM | Open batch<br>D:\Org\Data\VOA5975C\VG010422\VG010422_8260B.batch.bin                                                                                                                                                    |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 2/28/2022 1:49:23 PM | Set UserAnnotation = NI for compound Bromomethane in sample 04JAN10.D; previous value =                                                                                                                                 |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 2/28/2022 1:49:29 PM | Set UserAnnotation = GT for compound Chloroethane in sample 04JAN10.D; previous value =                                                                                                                                 |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 2/28/2022 1:49:34 PM | Set UserAnnotation = NI for compound 1,1-Dichloroethene in sample 04JAN10.D; previous value =                                                                                                                           |        |         | ✓       |           |



# Audit Trail report

| Name                          | User           | Time                 | Action                                                                                                                                                                                                            | Reason | Comment | Succeed | Exception |
|-------------------------------|----------------|----------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 2/28/2022 1:49:38 PM | Set UserAnnotation = NI for compound trans-1,2-Dichloroethene in sample 04JAN10.D; previous value =                                                                                                               |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 2/28/2022 1:49:43 PM | Set UserAnnotation = NI for compound Methyl tert-butyl ether (MTBE) in sample 04JAN10.D; previous value =                                                                                                         |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 2/28/2022 1:49:46 PM | Set UserAnnotation = NI for compound 2,2-Dichloropropane in sample 04JAN10.D; previous value =                                                                                                                    |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 2/28/2022 1:49:51 PM | Set UserAnnotation = NI for compound cis-1,2-Dichloroethene in sample 04JAN10.D; previous value =                                                                                                                 |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 2/28/2022 1:49:55 PM | Set UserAnnotation = NI for compound Bromochloromethane in sample 04JAN10.D; previous value =                                                                                                                     |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 2/28/2022 1:49:59 PM | Set UserAnnotation = NI for compound Dibromofluoromethane in sample 04JAN10.D; previous value =                                                                                                                   |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 2/28/2022 1:50:03 PM | Set UserAnnotation = NI for compound 1,2-Dichloroethane-d4 in sample 04JAN10.D; previous value =                                                                                                                  |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 2/28/2022 1:50:06 PM | Set UserAnnotation = NI for compound 1,2-Dichloroethane in sample 04JAN10.D; previous value =                                                                                                                     |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 2/28/2022 1:50:10 PM | Set UserAnnotation = NI for compound Trichloroethene in sample 04JAN10.D; previous value =                                                                                                                        |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 2/28/2022 1:50:14 PM | Set UserAnnotation = NI for compound Dibromomethane in sample 04JAN10.D; previous value =                                                                                                                         |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 2/28/2022 1:50:19 PM | Set UserAnnotation = NI for compound trans-1,3-Dichloropropene in sample 04JAN10.D; previous value =                                                                                                              |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 2/28/2022 1:50:23 PM | Set UserAnnotation = NI for compound 1,1,2-Trichloroethane in sample 04JAN10.D; previous value =                                                                                                                  |        |         | ✓       |           |
| CmdSaveBatchTable             | BL2000\mchavez | 2/28/2022 1:54:50 PM | Save batch<br>D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin                                                                                                                                 |        |         | ✓       |           |
| GenerateReport                | BL2000\mchavez | 2/28/2022 1:56:23 PM | Generates report - Method:<br>\\MASSHUNTER\Org\reports\LevelIV_Reports\Calibration\01_Init_Cal+Gen_Calibration+Gen_ResultsSummary.m,<br>Output Path:<br>D:\Org\Data\VOA5975C\VG010422\QuantReports\VG010422_8260B |        |         | ✓       |           |
| CmdStartMethodEditing         | BL2000\mchavez | 2/28/2022 1:57:20 PM | Start method editing                                                                                                                                                                                              |        |         | ✓       |           |

# Audit Trail report

| Name                       | User           | Time                 | Action                                                                                                                                                                                                              | Reason | Comment | Succeed | Exception |
|----------------------------|----------------|----------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdImportMethodFromFile    | BL2000\mchavez | 2/28/2022 1:57:21 PM | Import method from file<br>\\MASSHUNTER\Org\Data\Methods\Quant\VOA5975C\VOA5975C_010422_CAL\VOA5975C_8260B_SHT_DoD_L4_010422.m                                                                                      |        |         | ✓       |           |
| CmdApplyMethodToAllSamples | BL2000\mchavez | 2/28/2022 1:57:33 PM | Apply method to all samples                                                                                                                                                                                         |        |         | ✓       |           |
| CmdMethodClear             | BL2000\mchavez | 2/28/2022 1:57:33 PM | Clear method                                                                                                                                                                                                        |        |         | ✓       |           |
| CmdEndMethodEditing        | BL2000\mchavez | 2/28/2022 1:57:33 PM | End method editing                                                                                                                                                                                                  |        |         | ✓       |           |
| CmdQuantitate              | BL2000\mchavez | 2/28/2022 1:57:54 PM | Quantitate all compounds in all samples                                                                                                                                                                             |        |         | ✓       |           |
| CmdSaveBatchTable          | BL2000\mchavez | 2/28/2022 1:59:46 PM | Save batch<br>D:\Org\Data\VOA5975C\VG010422\QuantResults\VG010422_8260B.batch.bin                                                                                                                                   |        |         | ✓       |           |
| GenerateReport             | BL2000\mchavez | 2/28/2022 2:00:55 PM | Generates report - Method:<br>\\MASSHUNTER\Org\reports\LevelIV_Reports\Calibration\01_Init_Cal+Gen_Calibration+Gen_ResultsSummary.m,<br>Output Path:<br>D:\Org\Data\VOA5975C\VG010422\QuantReports\VG010422_8260B-1 |        |         | ✓       |           |

# Energy Laboratories Inc

# ANALYTICAL RUN Summary

02-Mar-22

Run ID VOA5975C.I\_220107A

|                                 |
|---------------------------------|
| <b>Run Start Date:</b> 1/7/2022 |
| <b>Analyst:</b> Melissa Chavez  |
| <b>Ical:</b>                    |
| <b>Column ID:</b>               |
| <b>Comments:</b>                |

| Std ID    | Std Name                                  | Std Amount | Std Units | Samp Amount | Samp Units | SampType   | Expiration Date |
|-----------|-------------------------------------------|------------|-----------|-------------|------------|------------|-----------------|
| VOCF3517  | Internal Standard / Surrogates (INT/SURR) | 8.4        | ul        | 42          | ml         | ALL (TUNE  | 12/31/2022      |
| VOCF3529B | 2nd Source MtBE                           | 1.05       | ul        | 42          | ml         | LCS, MS, M | 1/29/2022       |
| VOCF3546A | Liquids                                   | 1.05       | ul        | 42          | ml         | CCV        | 1/13/2022       |
| VOCF3549  | 2nd Source Ketones                        | 1.05       | ul        | 42          | ml         | LCS, MS, M | 1/15/2022       |
| VOCF3550  | Ketones                                   | 1.05       | ul        | 42          | ml         | CCV        | 1/16/2022       |
| VOCF3558B | 2nd Source Liquids                        | 1.05       | ul        | 42          | ml         | LCS, MS, M | 2/27/2022       |
| VOCF3559A | MtBE                                      | 1.05       | ul        | 42          | ml         | CCV        | 1/27/2022       |
| VOCF3562A | Gases                                     | 1.05       | ul        | 42          | ml         | CCV        | 1/10/2022       |
| VOCF3566A | 2nd Source Gases                          | 1.05       | ul        | 42          | ml         | LCS, MS, M | 1/11/2022       |

| Seq No             | Lab ID       | Test Code    | Sample Typ | File ID       | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |       |      |   |
|--------------------|--------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|-------|------|---|
| 14973448           | 07JAN02_D_TU | VOC-8260-BFB | TUNE       | DA5975C\VG010 | 1/7/2022 9:03:00 | 1     | R373037  |           | 0      | 0      |        |      |     |       |      |   |
| Analyte            | T            | Units        | RAW        | Final         | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH  | %RPD | Q |
| 173, % of mass 174 | A            | %            | 0          | 0             |                  | 100   | 0        | 0         | 0      | 0      | 0      | 0%   | 0   | 1.99  | 0%   |   |
| 174, % of mass 95  | A            | %            | 85.7       | 85.7          |                  | 100   | 0        | 0         | 0      | 0      | 0      | 86%  | 50  | 99.99 | 0%   |   |
| 175, % of mass 174 | A            | %            | 8.3        | 8.3           |                  | 100   | 0        | 0         | 0      | 0      | 0      | 8%   | 5   | 9     | 0%   |   |
| 176, % of mass 174 | A            | %            | 99.3       | 99.3          |                  | 100   | 0        | 0         | 0      | 0      | 0      | 99%  | 95  | 101   | 0%   |   |
| 177, % of mass 176 | A            | %            | 7.7        | 7.7           |                  | 100   | 0        | 0         | 0      | 0      | 0      | 8%   | 5   | 9     | 0%   |   |
| 50, % of mass 95   | A            | %            | 19.2       | 19.2          |                  | 100   | 0        | 0         | 0      | 0      | 0      | 19%  | 15  | 40    | 0%   |   |
| 75, % of mass 95   | A            | %            | 51.3       | 51.3          |                  | 100   | 0        | 0         | 0      | 0      | 0      | 51%  | 30  | 60    | 0%   |   |
| 95, Base Peak      | A            | %            | 100        | 100           |                  | 100   | 0        | 0         | 0      | 0      | 0      | 100% | 0   | 100   | 0%   |   |
| 96, % of mass 95   | A            | %            | 6.8        | 6.8           |                  | 100   | 0        | 0         | 0      | 0      | 0      | 7%   | 5   | 9     | 0%   |   |

| Seq No                    | Lab ID     | Test Code    | Sample Typ | File ID       | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|---------------------------|------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14973449                  | CCV010722_ | VOC-8260-W-Q | CCV        | DA5975CVVG010 | 1/7/2022 9:43:06 | 1     | R373037  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                   | T          | Units        | RAW        | Final         | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A          | ug/L         | 118.08544  | 4.7234176     |                  | 5     | 0        | 0         | 0.101  | 0.5    | 500    | 94%  | 80  | 120  | 0%   |   |
| 1,1,1-Trichloroethane     | A          | ug/L         | 125.09168  | 5.0036672     |                  | 5     | 0        | 0         | 0.131  | 0.5    | 500    | 100% | 80  | 120  | 0%   |   |
| 1,1,2,2-Tetrachloroethane | A          | ug/L         | 130.59813  | 5.2239252     |                  | 5     | 0        | 0         | 0.0872 | 0.5    | 500    | 104% | 80  | 120  | 0%   |   |
| 1,1,2-Trichloroethane     | A          | ug/L         | 123.52129  | 4.9408516     |                  | 5     | 0        | 0         | 0.108  | 0.5    | 500    | 99%  | 80  | 120  | 0%   |   |
| 1,1-Dichloroethane        | A          | ug/L         | 127.83306  | 5.1133224     |                  | 5     | 0        | 0         | 0.135  | 0.5    | 500    | 102% | 80  | 120  | 0%   |   |
| 1,1-Dichloroethene        | A          | ug/L         | 121.47259  | 4.8589036     |                  | 5     | 0        | 0         | 0.141  | 0.5    | 500    | 97%  | 80  | 120  | 0%   |   |
| 1,1-Dichloropropene       | A          | ug/L         | 125.60688  | 5.0242752     |                  | 5     | 0        | 0         | 0.083  | 0.5    | 500    | 100% | 80  | 120  | 0%   |   |
| 1,2,3-Trichloropropane    | A          | ug/L         | 129.90227  | 5.1960908     |                  | 5     | 0        | 0         | 0.235  | 0.5    | 500    | 104% | 80  | 120  | 0%   |   |
| 1,2-Dibromoethane         | A          | ug/L         | 125.22993  | 5.0091972     |                  | 5     | 0        | 0         | 0.0916 | 0.5    | 500    | 100% | 80  | 120  | 0%   |   |
| 1,2-Dichlorobenzene       | A          | ug/L         | 124.08023  | 4.9632092     |                  | 5     | 0        | 0         | 0.0746 | 0.5    | 500    | 99%  | 80  | 120  | 0%   |   |
| 1,2-Dichloroethane        | A          | ug/L         | 123.7158   | 4.948632      |                  | 5     | 0        | 0         | 0.116  | 0.5    | 500    | 99%  | 80  | 120  | 0%   |   |
| 1,2-Dichloropropane       | A          | ug/L         | 127.33164  | 5.0932656     |                  | 5     | 0        | 0         | 0.0847 | 0.5    | 500    | 102% | 80  | 120  | 0%   |   |
| 1,3-Dichlorobenzene       | A          | ug/L         | 124.85744  | 4.9942976     |                  | 5     | 0        | 0         | 0.0803 | 0.5    | 500    | 100% | 80  | 120  | 0%   |   |
| 1,3-Dichloropropane       | A          | ug/L         | 124.55548  | 4.9822192     |                  | 5     | 0        | 0         | 0.0791 | 0.5    | 500    | 100% | 80  | 120  | 0%   |   |
| 1,4-Dichlorobenzene       | A          | ug/L         | 126.09813  | 5.0439252     |                  | 5     | 0        | 0         | 0.0858 | 0.5    | 500    | 101% | 80  | 120  | 0%   |   |
| 2,2-Dichloropropane       | A          | ug/L         | 130.08225  | 5.20329       |                  | 5     | 0        | 0         | 0.186  | 0.5    | 500    | 104% | 80  | 120  | 0%   |   |
| 2-Chlorotoluene           | A          | ug/L         | 129.2634   | 5.170536      |                  | 5     | 0        | 0         | 0.0876 | 0.5    | 500    | 103% | 80  | 120  | 0%   |   |
| 4-Chlorotoluene           | A          | ug/L         | 132.69103  | 5.3076412     |                  | 5     | 0        | 0         | 0.0728 | 0.5    | 500    | 106% | 80  | 120  | 0%   |   |
| Benzene                   | A          | ug/L         | 127.07276  | 5.0829104     |                  | 5     | 0        | 0         | 0.0914 | 0.5    | 500    | 102% | 80  | 120  | 0%   |   |
| Bromobenzene              | A          | ug/L         | 130.11606  | 5.2046424     |                  | 5     | 0        | 0         | 0.0831 | 0.5    | 500    | 104% | 80  | 120  | 0%   |   |
| Bromochloromethane        | A          | ug/L         | 128.60244  | 5.1440976     |                  | 5     | 0        | 0         | 0.141  | 0.5    | 500    | 103% | 80  | 120  | 0%   |   |
| Bromodichloromethane      | A          | ug/L         | 123.9145   | 4.95658       |                  | 5     | 0        | 0         | 0.12   | 0.5    | 500    | 99%  | 80  | 120  | 0%   |   |
| Bromoform                 | A          | ug/L         | 128.72304  | 5.1489216     |                  | 5     | 0        | 0         | 0.119  | 0.5    | 500    | 103% | 80  | 120  | 0%   |   |
| Bromomethane              | A          | ug/L         | 132.28115  | 5.291246      |                  | 5     | 0        | 0         | 0.253  | 0.5    | 500    | 106% | 80  | 120  | 0%   |   |
| Carbon tetrachloride      | A          | ug/L         | 120.27745  | 4.811098      |                  | 5     | 0        | 0         | 0.143  | 0.5    | 500    | 96%  | 80  | 120  | 0%   |   |
| Chlorobenzene             | A          | ug/L         | 123.25086  | 4.9300344     |                  | 5     | 0        | 0         | 0.0914 | 0.5    | 500    | 99%  | 80  | 120  | 0%   |   |
| Chlorodibromomethane      | A          | ug/L         | 124.96785  | 4.998714      |                  | 5     | 0        | 0         | 0.0841 | 0.5    | 500    | 100% | 80  | 120  | 0%   |   |
| Chloroethane              | A          | ug/L         | 118.04495  | 4.721798      |                  | 5     | 0        | 0         | 0.169  | 0.5    | 500    | 94%  | 80  | 120  | 0%   |   |
| Chloroform                | A          | ug/L         | 121.57152  | 4.8628608     |                  | 5     | 0        | 0         | 0.0789 | 0.5    | 500    | 97%  | 80  | 120  | 0%   |   |
| Chloromethane             | A          | ug/L         | 116.39918  | 4.6559672     |                  | 5     | 0        | 0         | 0.162  | 0.5    | 500    | 93%  | 80  | 120  | 0%   |   |
| cis-1,2-Dichloroethene    | A          | ug/L         | 128.70764  | 5.1483056     |                  | 5     | 0        | 0         | 0.108  | 0.5    | 500    | 103% | 80  | 120  | 0%   |   |
| cis-1,3-Dichloropropene   | A          | ug/L         | 122.22136  | 4.8888544     |                  | 5     | 0        | 0         | 0.073  | 0.5    | 500    | 98%  | 80  | 120  | 0%   |   |
| Dibromomethane            | A          | ug/L         | 121.6934   | 4.867736      |                  | 5     | 0        | 0         | 0.147  | 0.5    | 500    | 97%  | 80  | 120  | 0%   |   |
| Dichlorodifluoromethane   | A          | ug/L         | 114.48502  | 4.5794008     |                  | 5     | 0        | 0         | 0.175  | 0.5    | 500    | 92%  | 80  | 120  | 0%   |   |
| Ethylbenzene              | A          | ug/L         | 123.92738  | 4.9570952     |                  | 5     | 0        | 0         | 0.0836 | 0.5    | 500    | 99%  | 80  | 120  | 0%   |   |

| Seq No                         | Lab ID     | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|--------------------------------|------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14973449                       | CCV010722_ | VOC-8260-W-Q | CCV        | DA5975C\VG010' | 1/7/2022 9:43:06 | 1     | R373037  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                        | T          | Units        | RAW        | Final          | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| m+p-Xylenes                    | A          | ug/L         | 252.2653   | 10.090612      |                  | 10    | 0        | 0         | 0.15   | 0.5    | 1000   | 101% | 80  | 120  | 0%   |   |
| Methyl ethyl ketone            | A          | ug/L         | 1257.21492 | 50.2885968     |                  | 50    | 0        | 0         | 1.77   | 10     | 5000   | 101% | 80  | 120  | 0%   |   |
| Methyl tert-butyl ether (MTBE) | A          | ug/L         | 127.82414  | 5.1129656      |                  | 5     | 0        | 0         | 0.101  | 0.5    | 500    | 102% | 80  | 120  | 0%   |   |
| Methylene chloride             | A          | ug/L         | 119.35881  | 4.7743524      |                  | 5     | 0        | 0         | 0.338  | 0.5    | 500    | 95%  | 80  | 120  | 0%   |   |
| o-Xylene                       | A          | ug/L         | 124.69512  | 4.9878048      |                  | 5     | 0        | 0         | 0.0604 | 0.5    | 500    | 100% | 80  | 120  | 0%   |   |
| Styrene                        | A          | ug/L         | 129.82914  | 5.1931656      |                  | 5     | 0        | 0         | 0.067  | 0.5    | 500    | 104% | 80  | 120  | 0%   |   |
| Tetrachloroethene              | A          | ug/L         | 117.83369  | 4.7133476      |                  | 5     | 0        | 0         | 0.0671 | 0.5    | 500    | 94%  | 80  | 120  | 0%   |   |
| Toluene                        | A          | ug/L         | 127.1937   | 5.087748       |                  | 5     | 0        | 0         | 0.0679 | 0.5    | 500    | 102% | 80  | 120  | 0%   |   |
| trans-1,2-Dichloroethene       | A          | ug/L         | 125.43198  | 5.0172792      |                  | 5     | 0        | 0         | 0.125  | 0.5    | 500    | 100% | 80  | 120  | 0%   |   |
| trans-1,3-Dichloropropene      | A          | ug/L         | 127.53024  | 5.1012096      |                  | 5     | 0        | 0         | 0.0846 | 0.5    | 500    | 102% | 80  | 120  | 0%   |   |
| Trichloroethene                | A          | ug/L         | 120.79095  | 4.831638       |                  | 5     | 0        | 0         | 0.0993 | 0.5    | 500    | 97%  | 80  | 120  | 0%   |   |
| Trichlorofluoromethane         | A          | ug/L         | 112.41757  | 4.4967028      |                  | 5     | 0        | 0         | 0.134  | 0.5    | 500    | 90%  | 80  | 120  | 0%   |   |
| Vinyl chloride                 | A          | ug/L         | 121.48241  | 4.8592964      |                  | 5     | 0        | 0         | 0.153  | 0.5    | 500    | 97%  | 80  | 120  | 0%   |   |
| 1,4-Dichlorobenzene-d4         | I          | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 0   | 0    | 0%   |   |
| Chlorobenzene-d5               | I          | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 0   | 0    | 0%   |   |
| Fluorobenzene                  | I          | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 0   | 0    | 0%   |   |
| Xylenes, Total                 | M          | ug/L         | 376.96042  | 15.0784168     |                  | 15    | 0        | 0         | 0.0604 | 0.5    | 1500   | 101% | 80  | 120  | 0%   |   |
| 1,2-Dichloroethane-d4          | S          | ug/L         | 280.59167  | 11.2236668     |                  | 10    | 0        | 0         | 0.229  | 0.5    | 500    | 112% | 80  | 120  | 0%   |   |
| Dibromofluoromethane           | S          | ug/L         | 279.46855  | 11.178742      |                  | 10    | 0        | 0         | 0.129  | 0.5    | 500    | 112% | 80  | 120  | 0%   |   |
| p-Bromofluorobenzene           | S          | ug/L         | 276.60604  | 11.0642416     |                  | 10    | 0        | 0         | 0.149  | 0.5    | 500    | 111% | 80  | 120  | 0%   |   |
| Toluene-d8                     | S          | ug/L         | 269.54488  | 10.7817952     |                  | 10    | 0        | 0         | 0.23   | 0.5    | 500    | 108% | 80  | 120  | 0%   |   |

| Seq No                    | Lab ID     | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|---------------------------|------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14973450                  | LCS010722_ | VOC-8260-W-Q | LCS-DOD    | DA5975C\VG010' | 1/7/2022 10:50:3 | 1     | R373037  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                   | T          | Units        | RAW        | Final          | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A          | ug/L         | 125.15027  | 5.0060108      |                  | 5     | 0        | 0         | 0.101  | 0.5    | 500    | 100% | 78  | 124  | 0%   |   |
| 1,1,1-Trichloroethane     | A          | ug/L         | 122.15451  | 4.8861804      |                  | 5     | 0        | 0         | 0.131  | 0.5    | 500    | 98%  | 74  | 131  | 0%   |   |
| 1,1,2,2-Tetrachloroethane | A          | ug/L         | 123.11919  | 4.9247676      |                  | 5     | 0        | 0         | 0.0872 | 0.5    | 500    | 98%  | 71  | 121  | 0%   |   |
| 1,1,2-Trichloroethane     | A          | ug/L         | 125.1597   | 5.006388       |                  | 5     | 0        | 0         | 0.108  | 0.5    | 500    | 100% | 80  | 119  | 0%   |   |
| 1,1-Dichloroethane        | A          | ug/L         | 131.07885  | 5.243154       |                  | 5     | 0        | 0         | 0.135  | 0.5    | 500    | 105% | 77  | 125  | 0%   |   |
| 1,1-Dichloroethene        | A          | ug/L         | 133.65174  | 5.3460696      |                  | 5     | 0        | 0         | 0.141  | 0.5    | 500    | 107% | 71  | 131  | 0%   |   |
| 1,1-Dichloropropene       | A          | ug/L         | 118.08273  | 4.7233092      |                  | 5     | 0        | 0         | 0.083  | 0.5    | 500    | 94%  | 79  | 125  | 0%   |   |
| 1,2,3-Trichloropropane    | A          | ug/L         | 125.17636  | 5.0070544      |                  | 5     | 0        | 0         | 0.235  | 0.5    | 500    | 100% | 73  | 125  | 0%   |   |
| 1,2-Dibromoethane         | A          | ug/L         | 123.15191  | 4.9260764      |                  | 5     | 0        | 0         | 0.0916 | 0.5    | 500    | 99%  | 78  | 122  | 0%   |   |

| Seq No                         | Lab ID     | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|--------------------------------|------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14973450                       | LCS010722_ | VOC-8260-W-Q | LCS-DOD    | DA5975C\VG010' | 1/7/2022 10:50:3 | 1     | R373037  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                        | T          | Units        | RAW        | Final          | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| 1,2-Dichlorobenzene            | A          | ug/L         | 125.55956  | 5.0223824      |                  | 5     | 0        | 0         | 0.0746 | 0.5    | 500    | 100% | 80  | 119  | 0%   |   |
| 1,2-Dichloroethane             | A          | ug/L         | 121.9792   | 4.879168       |                  | 5     | 0        | 0         | 0.116  | 0.5    | 500    | 98%  | 73  | 128  | 0%   |   |
| 1,2-Dichloropropane            | A          | ug/L         | 124.07441  | 4.9629764      |                  | 5     | 0        | 0         | 0.0847 | 0.5    | 500    | 99%  | 78  | 122  | 0%   |   |
| 1,3-Dichlorobenzene            | A          | ug/L         | 131.94939  | 5.2779756      |                  | 5     | 0        | 0         | 0.0803 | 0.5    | 500    | 106% | 80  | 119  | 0%   |   |
| 1,3-Dichloropropane            | A          | ug/L         | 121.38496  | 4.8553984      |                  | 5     | 0        | 0         | 0.0791 | 0.5    | 500    | 97%  | 80  | 119  | 0%   |   |
| 1,4-Dichlorobenzene            | A          | ug/L         | 128.63551  | 5.1454204      |                  | 5     | 0        | 0         | 0.0858 | 0.5    | 500    | 103% | 79  | 118  | 0%   |   |
| 2,2-Dichloropropane            | A          | ug/L         | 128.77441  | 5.1509764      |                  | 5     | 0        | 0         | 0.186  | 0.5    | 500    | 103% | 60  | 139  | 0%   |   |
| 2-Chlorotoluene                | A          | ug/L         | 130.04655  | 5.201862       |                  | 5     | 0        | 0         | 0.0876 | 0.5    | 500    | 104% | 79  | 122  | 0%   |   |
| 4-Chlorotoluene                | A          | ug/L         | 134.9812   | 5.399248       |                  | 5     | 0        | 0         | 0.0728 | 0.5    | 500    | 108% | 78  | 122  | 0%   |   |
| Benzene                        | A          | ug/L         | 127.6093   | 5.104372       |                  | 5     | 0        | 0         | 0.0914 | 0.5    | 500    | 102% | 79  | 120  | 0%   |   |
| Bromobenzene                   | A          | ug/L         | 131.56488  | 5.2625952      |                  | 5     | 0        | 0         | 0.0831 | 0.5    | 500    | 105% | 80  | 120  | 0%   |   |
| Bromochloromethane             | A          | ug/L         | 120.19576  | 4.8078304      |                  | 5     | 0        | 0         | 0.141  | 0.5    | 500    | 96%  | 78  | 123  | 0%   |   |
| Bromodichloromethane           | A          | ug/L         | 127.5739   | 5.102956       |                  | 5     | 0        | 0         | 0.12   | 0.5    | 500    | 102% | 79  | 125  | 0%   |   |
| Bromoform                      | A          | ug/L         | 131.15559  | 5.2462236      |                  | 5     | 0        | 0         | 0.119  | 0.5    | 500    | 105% | 66  | 130  | 0%   |   |
| Bromomethane                   | A          | ug/L         | 120.90262  | 4.8361048      |                  | 5     | 0        | 0         | 0.253  | 0.5    | 500    | 97%  | 53  | 141  | 0%   |   |
| Carbon tetrachloride           | A          | ug/L         | 117.63797  | 4.7055188      |                  | 5     | 0        | 0         | 0.143  | 0.5    | 500    | 94%  | 72  | 136  | 0%   |   |
| Chlorobenzene                  | A          | ug/L         | 125.64774  | 5.0259096      |                  | 5     | 0        | 0         | 0.0914 | 0.5    | 500    | 101% | 82  | 118  | 0%   |   |
| Chlorodibromomethane           | A          | ug/L         | 122.73184  | 4.9092736      |                  | 5     | 0        | 0         | 0.0841 | 0.5    | 500    | 98%  | 74  | 126  | 0%   |   |
| Chloroethane                   | A          | ug/L         | 109.6085   | 4.38434        |                  | 5     | 0        | 0         | 0.169  | 0.5    | 500    | 88%  | 60  | 138  | 0%   |   |
| Chloroform                     | A          | ug/L         | 119.37452  | 4.7749808      |                  | 5     | 0        | 0         | 0.0789 | 0.5    | 500    | 95%  | 79  | 124  | 0%   |   |
| Chloromethane                  | A          | ug/L         | 108.69779  | 4.3479116      |                  | 5     | 0        | 0         | 0.162  | 0.5    | 500    | 87%  | 50  | 139  | 0%   |   |
| cis-1,2-Dichloroethene         | A          | ug/L         | 129.68356  | 5.1873424      |                  | 5     | 0        | 0         | 0.108  | 0.5    | 500    | 104% | 78  | 123  | 0%   |   |
| cis-1,3-Dichloropropene        | A          | ug/L         | 117.25682  | 4.6902728      |                  | 5     | 0        | 0         | 0.073  | 0.5    | 500    | 94%  | 75  | 124  | 0%   |   |
| Dibromomethane                 | A          | ug/L         | 124.14929  | 4.9659716      |                  | 5     | 0        | 0         | 0.147  | 0.5    | 500    | 99%  | 79  | 123  | 0%   |   |
| Dichlorodifluoromethane        | A          | ug/L         | 103.63824  | 4.1455296      |                  | 5     | 0        | 0         | 0.175  | 0.5    | 500    | 83%  | 32  | 152  | 0%   |   |
| Ethylbenzene                   | A          | ug/L         | 125.94524  | 5.0378096      |                  | 5     | 0        | 0         | 0.0836 | 0.5    | 500    | 101% | 79  | 121  | 0%   |   |
| m+p-Xylenes                    | A          | ug/L         | 250.90789  | 10.0363156     |                  | 10    | 0        | 0         | 0.15   | 0.5    | 1000   | 100% | 80  | 121  | 0%   |   |
| Methyl ethyl ketone            | A          | ug/L         | 1138.31283 | 45.5325132     |                  | 50    | 0        | 0         | 1.77   | 10     | 5000   | 91%  | 56  | 143  | 0%   |   |
| Methyl tert-butyl ether (MTBE) | A          | ug/L         | 132.80502  | 5.3122008      |                  | 5     | 0        | 0         | 0.101  | 0.5    | 500    | 106% | 71  | 124  | 0%   |   |
| Methylene chloride             | A          | ug/L         | 118.10926  | 4.7243704      |                  | 5     | 0        | 0         | 0.338  | 0.5    | 500    | 94%  | 74  | 124  | 0%   |   |
| o-Xylene                       | A          | ug/L         | 129.8994   | 5.195976       |                  | 5     | 0        | 0         | 0.0604 | 0.5    | 500    | 104% | 78  | 122  | 0%   |   |
| Styrene                        | A          | ug/L         | 132.51502  | 5.3006008      |                  | 5     | 0        | 0         | 0.067  | 0.5    | 500    | 106% | 78  | 123  | 0%   |   |
| Tetrachloroethene              | A          | ug/L         | 118.88372  | 4.7553488      |                  | 5     | 0        | 0         | 0.0671 | 0.5    | 500    | 95%  | 74  | 129  | 0%   |   |
| Toluene                        | A          | ug/L         | 129.15194  | 5.1660776      |                  | 5     | 0        | 0         | 0.0679 | 0.5    | 500    | 103% | 80  | 121  | 0%   |   |
| trans-1,2-Dichloroethene       | A          | ug/L         | 129.83201  | 5.1932804      |                  | 5     | 0        | 0         | 0.125  | 0.5    | 500    | 104% | 75  | 124  | 0%   |   |

| Seq No                    | Lab ID     | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|---------------------------|------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14973450                  | LCS010722_ | VOC-8260-W-Q | LCS-DOD    | DA5975C\VG010' | 1/7/2022 10:50:3 | 1     | R373037  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                   | T          | Units        | RAW        | Final          | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| trans-1,3-Dichloropropene | A          | ug/L         | 131.25712  | 5.2502848      |                  | 5     | 0        | 0         | 0.0846 | 0.5    | 500    | 105% | 73  | 127  | 0%   |   |
| Trichloroethene           | A          | ug/L         | 125.89894  | 5.0359576      |                  | 5     | 0        | 0         | 0.0993 | 0.5    | 500    | 101% | 79  | 123  | 0%   |   |
| Trichlorofluoromethane    | A          | ug/L         | 112.75149  | 4.5100596      |                  | 5     | 0        | 0         | 0.134  | 0.5    | 500    | 90%  | 65  | 141  | 0%   |   |
| Vinyl chloride            | A          | ug/L         | 119.23499  | 4.7693996      |                  | 5     | 0        | 0         | 0.153  | 0.5    | 500    | 95%  | 58  | 137  | 0%   |   |
| 1,4-Dichlorobenzene-d4    | I          | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 0   | 0    | 0%   |   |
| Chlorobenzene-d5          | I          | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 0   | 0    | 0%   |   |
| Fluorobenzene             | I          | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 0   | 0    | 0%   |   |
| Xylenes, Total            | M          | ug/L         | 380.80729  | 15.2322916     |                  | 15    | 0        | 0         | 0.0604 | 0.5    | 1500   | 102% | 79  | 121  | 0%   |   |
| 1,2-Dichloroethane-d4     | S          | ug/L         | 282.91531  | 11.3166124     |                  | 10    | 0        | 0         | 0.229  | 0.5    | 500    | 113% | 81  | 118  | 0%   |   |
| Dibromofluoromethane      | S          | ug/L         | 270.45155  | 10.818062      |                  | 10    | 0        | 0         | 0.129  | 0.5    | 500    | 108% | 80  | 119  | 0%   |   |
| p-Bromofluorobenzene      | S          | ug/L         | 271.98175  | 10.87927       |                  | 10    | 0        | 0         | 0.149  | 0.5    | 500    | 109% | 85  | 114  | 0%   |   |
| Toluene-d8                | S          | ug/L         | 271.05199  | 10.8420796     |                  | 10    | 0        | 0         | 0.23   | 0.5    | 500    | 108% | 89  | 112  | 0%   |   |

| Seq No                    | Lab ID      | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|---------------------------|-------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14973453                  | MBLK010722_ | VOC-8260-W-Q | MBLK       | DA5975C\VG010' | 1/7/2022 11:45:0 | 1     | R373037  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                   | T           | Units        | RAW        | Final          | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A           | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.101  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 1,1,1-Trichloroethane     | A           | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.131  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 1,1,2,2-Tetrachloroethane | A           | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0872 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 1,1,2-Trichloroethane     | A           | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.108  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 1,1-Dichloroethane        | A           | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.135  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 1,1-Dichloroethene        | A           | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.141  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 1,1-Dichloropropene       | A           | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.083  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 1,2,3-Trichloropropane    | A           | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.235  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 1,2-Dibromoethane         | A           | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0916 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 1,2-Dichlorobenzene       | A           | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0746 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 1,2-Dichloroethane        | A           | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.116  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 1,2-Dichloropropane       | A           | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0847 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 1,3-Dichlorobenzene       | A           | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0803 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 1,3-Dichloropropane       | A           | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0791 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 1,4-Dichlorobenzene       | A           | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0858 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 2,2-Dichloropropane       | A           | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.186  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 2-Chlorotoluene           | A           | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0876 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 4-Chlorotoluene           | A           | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0728 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |

| Seq No                         | Lab ID      | Test Code    | Sample Typ | File ID       | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|--------------------------------|-------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14973453                       | MBLK010722_ | VOC-8260-W-Q | MBLK       | DA5975CVVG010 | 1/7/2022 11:45:0 | 1     | R373037  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                        | T           | Units        | RAW        | Final         | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| Benzene                        | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0914 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Bromobenzene                   | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0831 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Bromochloromethane             | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.141  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Bromodichloromethane           | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.12   | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Bromoform                      | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.119  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Bromomethane                   | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.253  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Carbon tetrachloride           | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.143  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Chlorobenzene                  | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0914 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Chlorodibromomethane           | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0841 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Chloroethane                   | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.169  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Chloroform                     | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0789 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Chloromethane                  | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.162  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| cis-1,2-Dichloroethene         | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.108  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| cis-1,3-Dichloropropene        | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.073  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Dibromomethane                 | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.147  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Dichlorodifluoromethane        | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.175  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Ethylbenzene                   | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0836 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| m+p-Xylenes                    | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.15   | 0.5    | 1000   | 0%   | 0   | 0    | 0%   |   |
| Methyl ethyl ketone            | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 1.77   | 10     | 5000   | 0%   | 0   | 0    | 0%   |   |
| Methyl tert-butyl ether (MTBE) | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.101  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Methylene chloride             | A           | ug/L         | 1.28894    | 0             |                  | 0     | 0        | 0         | 0.338  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| o-Xylene                       | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0604 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Styrene                        | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.067  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Tetrachloroethene              | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0671 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Toluene                        | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0679 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| trans-1,2-Dichloroethene       | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.125  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| trans-1,3-Dichloropropene      | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0846 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Trichloroethene                | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0993 | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Trichlorofluoromethane         | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.134  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| Vinyl chloride                 | A           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.153  | 0.5    | 500    | 0%   | 0   | 0    | 0%   |   |
| 1,4-Dichlorobenzene-d4         | I           | ug/L         | 250        | 10            |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 0   | 0    | 0%   |   |
| Chlorobenzene-d5               | I           | ug/L         | 250        | 10            |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 0   | 0    | 0%   |   |
| Fluorobenzene                  | I           | ug/L         | 250        | 10            |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 0   | 0    | 0%   |   |
| Xylenes, Total                 | M           | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0604 | 0.5    | 1500   | 0%   | 0   | 0    | 0%   |   |
| 1,2-Dichloroethane-d4          | S           | ug/L         | 279.14576  | 11.1658304    |                  | 10    | 0        | 0         | 0.229  | 0.5    | 500    | 112% | 81  | 118  | 0%   |   |



| Seq No               | Lab ID      | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|----------------------|-------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14973453             | MBLK010722_ | VOC-8260-W-Q | MBLK       | DA5975C\VG010' | 1/7/2022 11:45:0 | 1     | R373037  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte              | T           | Units        | RAW        | Final          | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| Dibromofluoromethane | S           | ug/L         | 270.76663  | 10.8306652     |                  | 10    | 0        | 0         | 0.129  | 0.5    | 500    | 108% | 80  | 119  | 0%   |   |
| p-Bromofluorobenzene | S           | ug/L         | 274.98941  | 10.9995764     |                  | 10    | 0        | 0         | 0.149  | 0.5    | 500    | 110% | 85  | 114  | 0%   |   |
| Toluene-d8           | S           | ug/L         | 264.37748  | 10.5750992     |                  | 10    | 0        | 0         | 0.23   | 0.5    | 500    | 106% | 89  | 112  | 0%   |   |

| Seq No                    | Lab ID        | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|---------------------------|---------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14973457                  | B22010214-002 | VOC-8260-W-S | SAMP       | DA5975C\VG010' | 1/7/2022 12:24:5 | 1     | R373037  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                   | T             | Units        | RAW        | Final          | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.101  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1,1-Trichloroethane     | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.131  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1,2,2-Tetrachloroethane | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0872 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1,2-Trichloroethane     | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.108  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1-Dichloroethane        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.135  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1-Dichloroethene        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.141  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1-Dichloropropene       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.083  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2,3-Trichloropropane    | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.235  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2-Dibromoethane         | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0916 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2-Dichlorobenzene       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0746 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2-Dichloroethane        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.116  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2-Dichloropropane       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0847 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,3-Dichlorobenzene       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0803 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,3-Dichloropropane       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0791 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,4-Dichlorobenzene       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0858 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 2,2-Dichloropropane       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.186  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 2-Chlorotoluene           | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0876 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 4-Chlorotoluene           | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0728 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Benzene                   | A             | ug/L         | 0.048      | 0              |                  | 0     | 0        | 0         | 0.0914 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Bromobenzene              | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0831 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Bromochloromethane        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.141  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Bromodichloromethane      | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.12   | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Bromoform                 | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.119  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Bromomethane              | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.253  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Carbon tetrachloride      | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.143  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Chlorobenzene             | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0914 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Chlorodibromomethane      | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0841 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |

| Seq No                         | Lab ID        | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|--------------------------------|---------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14973457                       | B22010214-002 | VOC-8260-W-S | SAMP       | DA5975C\VG010' | 1/7/2022 12:24:5 | 1     | R373037  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                        | T             | Units        | RAW        | Final          | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| Chloroethane                   | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.169  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Chloroform                     | A             | ug/L         | 0.14554    | 0              |                  | 0     | 0        | 0         | 0.0789 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Chloromethane                  | A             | ug/L         | 1.44449    | 0              |                  | 0     | 0        | 0         | 0.162  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| cis-1,2-Dichloroethene         | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.108  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| cis-1,3-Dichloropropene        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.073  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Dibromomethane                 | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.147  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Dichlorodifluoromethane        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.175  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Ethylbenzene                   | A             | ug/L         | 0.10634    | 0              |                  | 0     | 0        | 0         | 0.0836 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| m+p-Xylenes                    | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.15   | 1      | 1000   | 0%   | 0   | 0    | 0%   | U |
| Methyl ethyl ketone            | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 1.77   | 20     | 5000   | 0%   | 0   | 0    | 0%   | U |
| Methyl tert-butyl ether (MTBE) | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.101  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Methylene chloride             | A             | ug/L         | 1.98693    | 0              |                  | 0     | 0        | 0         | 0.338  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| o-Xylene                       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0604 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Styrene                        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.067  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Tetrachloroethene              | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0671 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Toluene                        | A             | ug/L         | 1.99774    | 0.0799096      |                  | 0     | 0        | 0         | 0.0679 | 1      | 500    | 0%   | 0   | 0    | 0%   | J |
| trans-1,2-Dichloroethene       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.125  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| trans-1,3-Dichloropropene      | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0846 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Trichloroethene                | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0993 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Trichlorofluoromethane         | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.134  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Vinyl chloride                 | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.153  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,4-Dichlorobenzene-d4         | I             | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0      | 0      | 0      | 0%   | 0   | 0    | 0%   |   |
| Chlorobenzene-d5               | I             | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0.1    | 0      | 0      | 0%   | 0   | 0    | 0%   |   |
| Fluorobenzene                  | I             | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0.1    | 0      | 0      | 0%   | 0   | 0    | 0%   |   |
| Xylenes, Total                 | M             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0604 | 1      | 0      | 0%   | 0   | 0    | 0%   | U |
| 1,2-Dichloroethane-d4          | S             | ug/L         | 314.75492  | 12.5901968     |                  | 10    | 0        | 0         | 0.229  | 1      | 500    | 126% | 81  | 118  | 0%   | S |
| Dibromofluoromethane           | S             | ug/L         | 292.59389  | 11.7037556     |                  | 10    | 0        | 0         | 0.129  | 1      | 500    | 117% | 80  | 119  | 0%   |   |
| p-Bromofluorobenzene           | S             | ug/L         | 283.55508  | 11.3422032     |                  | 10    | 0        | 0         | 0.149  | 1      | 500    | 113% | 85  | 114  | 0%   |   |
| Toluene-d8                     | S             | ug/L         | 260.0307   | 10.401228      |                  | 10    | 0        | 0         | 0.23   | 1      | 500    | 104% | 89  | 112  | 0%   |   |

| Seq No   | Lab ID        | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|----------|---------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14973458 | B22010219-002 | VOC-8260-W-S | SAMP       | DA5975C\VG010' | 1/7/2022 12:52:1 | 1     | R373037  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte  | T             | Units        | RAW        | Final          | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |

| Seq No                    | Lab ID        | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|---------------------------|---------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14973458                  | B22010219-002 | VOC-8260-W-S | SAMP       | DA5975C\VG010' | 1/7/2022 12:52:1 | 1     | R373037  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                   | T             | Units        | RAW        | Final          | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.101  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1,1-Trichloroethane     | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.131  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1,2,2-Tetrachloroethane | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0872 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1,2-Trichloroethane     | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.108  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1-Dichloroethane        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.135  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1-Dichloroethene        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.141  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1-Dichloropropene       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.083  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2,3-Trichloropropane    | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.235  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2-Dibromoethane         | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0916 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2-Dichlorobenzene       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0746 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2-Dichloroethane        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.116  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2-Dichloropropane       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0847 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,3-Dichlorobenzene       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0803 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,3-Dichloropropane       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0791 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,4-Dichlorobenzene       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0858 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 2,2-Dichloropropane       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.186  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 2-Chlorotoluene           | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0876 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 4-Chlorotoluene           | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0728 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Benzene                   | A             | ug/L         | 0.06481    | 0              |                  | 0     | 0        | 0         | 0.0914 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Bromobenzene              | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0831 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Bromochloromethane        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.141  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Bromodichloromethane      | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.12   | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Bromoform                 | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.119  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Bromomethane              | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.253  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Carbon tetrachloride      | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.143  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Chlorobenzene             | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0914 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Chlorodibromomethane      | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0841 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Chloroethane              | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.169  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Chloroform                | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0789 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Chloromethane             | A             | ug/L         | 1.90607    | 0              |                  | 0     | 0        | 0         | 0.162  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| cis-1,2-Dichloroethene    | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.108  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| cis-1,3-Dichloropropene   | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.073  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Dibromomethane            | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.147  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Dichlorodifluoromethane   | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.175  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Ethylbenzene              | A             | ug/L         | 0.12145    | 0              |                  | 0     | 0        | 0         | 0.0836 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |

| Seq No                         | Lab ID        | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|--------------------------------|---------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14973458                       | B22010219-002 | VOC-8260-W-S | SAMP       | DA5975C\VG010' | 1/7/2022 12:52:1 | 1     | R373037  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                        | T             | Units        | RAW        | Final          | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| m+p-Xylenes                    | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.15   | 1      | 1000   | 0%   | 0   | 0    | 0%   | U |
| Methyl ethyl ketone            | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 1.77   | 20     | 5000   | 0%   | 0   | 0    | 0%   | U |
| Methyl tert-butyl ether (MTBE) | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.101  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Methylene chloride             | A             | ug/L         | 1.833      | 0              |                  | 0     | 0        | 0         | 0.338  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| o-Xylene                       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0604 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Styrene                        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.067  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Tetrachloroethene              | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0671 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Toluene                        | A             | ug/L         | 1.80909    | 0.0723636      |                  | 0     | 0        | 0         | 0.0679 | 1      | 500    | 0%   | 0   | 0    | 0%   | J |
| trans-1,2-Dichloroethene       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.125  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| trans-1,3-Dichloropropene      | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0846 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Trichloroethene                | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0993 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Trichlorofluoromethane         | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.134  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Vinyl chloride                 | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.153  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,4-Dichlorobenzene-d4         | I             | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0      | 0      | 0      | 0%   | 0   | 0    | 0%   |   |
| Chlorobenzene-d5               | I             | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0.1    | 0      | 0      | 0%   | 0   | 0    | 0%   |   |
| Fluorobenzene                  | I             | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0.1    | 0      | 0      | 0%   | 0   | 0    | 0%   |   |
| Xylenes, Total                 | M             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0604 | 1      | 0      | 0%   | 0   | 0    | 0%   | U |
| 1,2-Dichloroethane-d4          | S             | ug/L         | 289.53136  | 11.5812544     |                  | 10    | 0        | 0         | 0.229  | 1      | 500    | 116% | 81  | 118  | 0%   |   |
| Dibromofluoromethane           | S             | ug/L         | 275.67606  | 11.0270424     |                  | 10    | 0        | 0         | 0.129  | 1      | 500    | 110% | 80  | 119  | 0%   |   |
| p-Bromofluorobenzene           | S             | ug/L         | 279.27018  | 11.1708072     |                  | 10    | 0        | 0         | 0.149  | 1      | 500    | 112% | 85  | 114  | 0%   |   |
| Toluene-d8                     | S             | ug/L         | 263.89535  | 10.555814      |                  | 10    | 0        | 0         | 0.23   | 1      | 500    | 106% | 89  | 112  | 0%   |   |

| Seq No                    | Lab ID        | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|---------------------------|---------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14973459                  | B22010262-002 | VOC-8260-W-S | SAMP       | DA5975C\VG010' | 1/7/2022 1:19:35 | 1     | R373037  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                   | T             | Units        | RAW        | Final          | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.101  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1,1-Trichloroethane     | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.131  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1,2,2-Tetrachloroethane | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0872 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1,2-Trichloroethane     | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.108  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1-Dichloroethane        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.135  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1-Dichloroethene        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.141  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1-Dichloropropene       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.083  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2,3-Trichloropropane    | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.235  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2-Dibromoethane         | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0916 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |

| Seq No                         | Lab ID        | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|--------------------------------|---------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14973459                       | B22010262-002 | VOC-8260-W-S | SAMP       | DA5975C\VG010' | 1/7/2022 1:19:35 | 1     | R373037  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                        | T             | Units        | RAW        | Final          | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| 1,2-Dichlorobenzene            | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0746 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2-Dichloroethane             | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.116  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2-Dichloropropane            | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0847 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,3-Dichlorobenzene            | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0803 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,3-Dichloropropane            | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0791 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,4-Dichlorobenzene            | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0858 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 2,2-Dichloropropane            | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.186  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 2-Chlorotoluene                | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0876 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 4-Chlorotoluene                | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0728 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Benzene                        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0914 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Bromobenzene                   | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0831 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Bromochloromethane             | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.141  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Bromodichloromethane           | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.12   | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Bromoform                      | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.119  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Bromomethane                   | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.253  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Carbon tetrachloride           | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.143  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Chlorobenzene                  | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0914 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Chlorodibromomethane           | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0841 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Chloroethane                   | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.169  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Chloroform                     | A             | ug/L         | 0.24661    | 0              |                  | 0     | 0        | 0         | 0.0789 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Chloromethane                  | A             | ug/L         | 0.80639    | 0              |                  | 0     | 0        | 0         | 0.162  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| cis-1,2-Dichloroethene         | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.108  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| cis-1,3-Dichloropropene        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.073  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Dibromomethane                 | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.147  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Dichlorodifluoromethane        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.175  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Ethylbenzene                   | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0836 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| m+p-Xylenes                    | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.15   | 1      | 1000   | 0%   | 0   | 0    | 0%   | U |
| Methyl ethyl ketone            | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 1.77   | 20     | 5000   | 0%   | 0   | 0    | 0%   | U |
| Methyl tert-butyl ether (MTBE) | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.101  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Methylene chloride             | A             | ug/L         | 2.20608    | 0              |                  | 0     | 0        | 0         | 0.338  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| o-Xylene                       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0604 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Styrene                        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.067  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Tetrachloroethene              | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0671 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Toluene                        | A             | ug/L         | 2.19497    | 0.0877988      |                  | 0     | 0        | 0         | 0.0679 | 1      | 500    | 0%   | 0   | 0    | 0%   | J |
| trans-1,2-Dichloroethene       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.125  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |

| Seq No                    | Lab ID        | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|---------------------------|---------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14973459                  | B22010262-002 | VOC-8260-W-S | SAMP       | DA5975C\VG010' | 1/7/2022 1:19:35 | 1     | R373037  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                   | T             | Units        | RAW        | Final          | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| trans-1,3-Dichloropropene | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0846 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Trichloroethene           | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0993 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Trichlorofluoromethane    | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.134  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Vinyl chloride            | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.153  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,4-Dichlorobenzene-d4    | I             | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0      | 0      | 0      | 0%   | 0   | 0    | 0%   |   |
| Chlorobenzene-d5          | I             | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0.1    | 0      | 0      | 0%   | 0   | 0    | 0%   |   |
| Fluorobenzene             | I             | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0.1    | 0      | 0      | 0%   | 0   | 0    | 0%   |   |
| Xylenes, Total            | M             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0604 | 1      | 0      | 0%   | 0   | 0    | 0%   | U |
| 1,2-Dichloroethane-d4     | S             | ug/L         | 281.55972  | 11.2623888     |                  | 10    | 0        | 0         | 0.229  | 1      | 500    | 113% | 81  | 118  | 0%   |   |
| Dibromofluoromethane      | S             | ug/L         | 277.07768  | 11.0831072     |                  | 10    | 0        | 0         | 0.129  | 1      | 500    | 111% | 80  | 119  | 0%   |   |
| p-Bromofluorobenzene      | S             | ug/L         | 270.77107  | 10.8308428     |                  | 10    | 0        | 0         | 0.149  | 1      | 500    | 108% | 85  | 114  | 0%   |   |
| Toluene-d8                | S             | ug/L         | 271.91357  | 10.8765428     |                  | 10    | 0        | 0         | 0.23   | 1      | 500    | 109% | 89  | 112  | 0%   |   |

| Seq No   | Lab ID        | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|----------|---------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14973460 | B22010214-002 | VOC-8260-W-S | SAMP       | DA5975C\VG010' | 1/7/2022 1:46:47 | 1     | R373037  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte  | T             | Units        | RAW        | Final          | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |

| Seq No                    | Lab ID        | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|---------------------------|---------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14973461                  | B22010219-001 | VOC-8260-W-S | SAMP       | DA5975C\VG010' | 1/7/2022 2:14:04 | 1     | R373037  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                   | T             | Units        | RAW        | Final          | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.101  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1,1-Trichloroethane     | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.131  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1,2,2-Tetrachloroethane | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0872 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1,2-Trichloroethane     | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.108  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1-Dichloroethane        | A             | ug/L         | 0.6175     | 0              |                  | 0     | 0        | 0         | 0.135  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1-Dichloroethene        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.141  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1-Dichloropropene       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.083  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2,3-Trichloropropane    | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.235  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2-Dibromoethane         | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0916 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2-Dichlorobenzene       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0746 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2-Dichloroethane        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.116  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2-Dichloropropane       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0847 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |

| Seq No                         | Lab ID        | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |    |
|--------------------------------|---------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|----|
| 14973461                       | B22010219-001 | VOC-8260-W-S | SAMP       | DA5975CVVG010' | 1/7/2022 2:14:04 | 1     | R373037  |           | 0      | 0      |        |      |     |      |      |    |
| Analyte                        | T             | Units        | RAW        | Final          | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q  |
| 1,3-Dichlorobenzene            | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0803 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| 1,3-Dichloropropane            | A             | ug/L         | 0.40048    | 0              |                  | 0     | 0        | 0         | 0.0791 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| 1,4-Dichlorobenzene            | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0858 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| 2,2-Dichloropropane            | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.186  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| 2-Chlorotoluene                | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0876 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| 4-Chlorotoluene                | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0728 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Benzene                        | A             | ug/L         | 0.43706    | 0              |                  | 0     | 0        | 0         | 0.0914 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Bromobenzene                   | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0831 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Bromochloromethane             | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.141  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Bromodichloromethane           | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.12   | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Bromoform                      | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.119  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Bromomethane                   | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.253  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Carbon tetrachloride           | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.143  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Chlorobenzene                  | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0914 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Chlorodibromomethane           | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0841 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Chloroethane                   | A             | ug/L         | 2.80665    | 0              |                  | 0     | 0        | 0         | 0.169  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Chloroform                     | A             | ug/L         | 0.50573    | 0              |                  | 0     | 0        | 0         | 0.0789 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Chloromethane                  | A             | ug/L         | 1.01509    | 0              |                  | 0     | 0        | 0         | 0.162  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| cis-1,2-Dichloroethene         | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.108  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| cis-1,3-Dichloropropene        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.073  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Dibromomethane                 | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.147  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Dichlorodifluoromethane        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.175  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Ethylbenzene                   | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0836 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| m+p-Xylenes                    | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.15   | 1      | 1000   | 0%   | 0   | 0    | 0%   | U  |
| Methyl ethyl ketone            | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 1.77   | 20     | 5000   | 0%   | 0   | 0    | 0%   | U  |
| Methyl tert-butyl ether (MTBE) | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.101  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Methylene chloride             | A             | ug/L         | 1.07273    | 0              |                  | 0     | 0        | 0         | 0.338  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| o-Xylene                       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0604 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Styrene                        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.067  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Tetrachloroethene              | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0671 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Toluene                        | A             | ug/L         | 0.34358    | 0              |                  | 0     | 0        | 0         | 0.0679 | 1      | 500    | 0%   | 0   | 0    | 0%   | UT |
| trans-1,2-Dichloroethene       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.125  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| trans-1,3-Dichloropropene      | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0846 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Trichloroethene                | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0993 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Trichlorofluoromethane         | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.134  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |

| Seq No                 | Lab ID        | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|------------------------|---------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14973461               | B22010219-001 | VOC-8260-W-S | SAMP       | DA5975C\VG010' | 1/7/2022 2:14:04 | 1     | R373037  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                | T             | Units        | RAW        | Final          | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| Vinyl chloride         | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.153  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,4-Dichlorobenzene-d4 | I             | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0      | 0      | 0      | 0%   | 0   | 0    | 0%   |   |
| Chlorobenzene-d5       | I             | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0.1    | 0      | 0      | 0%   | 0   | 0    | 0%   |   |
| Fluorobenzene          | I             | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0.1    | 0      | 0      | 0%   | 0   | 0    | 0%   |   |
| Xylenes, Total         | M             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0604 | 1      | 0      | 0%   | 0   | 0    | 0%   | U |
| 1,2-Dichloroethane-d4  | S             | ug/L         | 295.01742  | 11.8006968     |                  | 10    | 0        | 0         | 0.229  | 1      | 500    | 118% | 81  | 118  | 0%   |   |
| Dibromofluoromethane   | S             | ug/L         | 277.84253  | 11.1137012     |                  | 10    | 0        | 0         | 0.129  | 1      | 500    | 111% | 80  | 119  | 0%   |   |
| p-Bromofluorobenzene   | S             | ug/L         | 270.69927  | 10.8279708     |                  | 10    | 0        | 0         | 0.149  | 1      | 500    | 108% | 85  | 114  | 0%   |   |
| Toluene-d8             | S             | ug/L         | 269.72701  | 10.7890804     |                  | 10    | 0        | 0         | 0.23   | 1      | 500    | 108% | 89  | 112  | 0%   |   |

| Seq No                    | Lab ID        | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|---------------------------|---------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14973462                  | B22010213-002 | VOC-8260-W-S | SAMP       | DA5975C\VG010' | 1/7/2022 2:41:20 | 1     | R373037  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                   | T             | Units        | RAW        | Final          | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.101  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1,1-Trichloroethane     | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.131  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1,2,2-Tetrachloroethane | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0872 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1,2-Trichloroethane     | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.108  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1-Dichloroethane        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.135  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1-Dichloroethene        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.141  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1-Dichloropropene       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.083  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2,3-Trichloropropane    | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.235  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2-Dibromoethane         | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0916 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2-Dichlorobenzene       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0746 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2-Dichloroethane        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.116  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2-Dichloropropane       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0847 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,3-Dichlorobenzene       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0803 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,3-Dichloropropane       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0791 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,4-Dichlorobenzene       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0858 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 2,2-Dichloropropane       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.186  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 2-Chlorotoluene           | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0876 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 4-Chlorotoluene           | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0728 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Benzene                   | A             | ug/L         | 0.12888    | 0              |                  | 0     | 0        | 0         | 0.0914 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Bromobenzene              | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0831 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Bromochloromethane        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.141  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |



| Seq No                         | Lab ID        | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |    |
|--------------------------------|---------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|----|
| 14973462                       | B22010213-002 | VOC-8260-W-S | SAMP       | DA5975C\VG010' | 1/7/2022 2:41:20 | 1     | R373037  |           | 0      | 0      |        |      |     |      |      |    |
| Analyte                        | T             | Units        | RAW        | Final          | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q  |
| Bromodichloromethane           | A             | ug/L         | 0.66597    | 0              |                  | 0     | 0        | 0         | 0.12   | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Bromoform                      | A             | ug/L         | 6.9642     | 0.278568       |                  | 0     | 0        | 0         | 0.119  | 1      | 500    | 0%   | 0   | 0    | 0%   | J  |
| Bromomethane                   | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.253  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Carbon tetrachloride           | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.143  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Chlorobenzene                  | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0914 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Chlorodibromomethane           | A             | ug/L         | 2.48888    | 0.0995552      |                  | 0     | 0        | 0         | 0.0841 | 1      | 500    | 0%   | 0   | 0    | 0%   | J  |
| Chloroethane                   | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.169  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Chloroform                     | A             | ug/L         | 1.08961    | 0              |                  | 0     | 0        | 0         | 0.0789 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Chloromethane                  | A             | ug/L         | 0.67305    | 0              |                  | 0     | 0        | 0         | 0.162  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| cis-1,2-Dichloroethene         | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.108  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| cis-1,3-Dichloropropene        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.073  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Dibromomethane                 | A             | ug/L         | 0.31217    | 0              |                  | 0     | 0        | 0         | 0.147  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Dichlorodifluoromethane        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.175  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Ethylbenzene                   | A             | ug/L         | 0.36732    | 0              |                  | 0     | 0        | 0         | 0.0836 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| m+p-Xylenes                    | A             | ug/L         | 0.88259    | 0              |                  | 0     | 0        | 0         | 0.15   | 1      | 1000   | 0%   | 0   | 0    | 0%   | U  |
| Methyl ethyl ketone            | A             | ug/L         | 5.01792    | 0              |                  | 0     | 0        | 0         | 1.77   | 20     | 5000   | 0%   | 0   | 0    | 0%   | U  |
| Methyl tert-butyl ether (MTBE) | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.101  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Methylene chloride             | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.338  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| o-Xylene                       | A             | ug/L         | 2.80675    | 0.11227        |                  | 0     | 0        | 0         | 0.0604 | 1      | 500    | 0%   | 0   | 0    | 0%   | J  |
| Styrene                        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.067  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Tetrachloroethene              | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0671 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Toluene                        | A             | ug/L         | 0.23877    | 0              |                  | 0     | 0        | 0         | 0.0679 | 1      | 500    | 0%   | 0   | 0    | 0%   | UT |
| trans-1,2-Dichloroethene       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.125  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| trans-1,3-Dichloropropene      | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0846 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Trichloroethene                | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0993 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Trichlorofluoromethane         | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.134  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Vinyl chloride                 | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.153  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| 1,4-Dichlorobenzene-d4         | I             | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0      | 0      | 0      | 0%   | 0   | 0    | 0%   |    |
| Chlorobenzene-d5               | I             | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0.1    | 0      | 0      | 0%   | 0   | 0    | 0%   |    |
| Fluorobenzene                  | I             | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0.1    | 0      | 0      | 0%   | 0   | 0    | 0%   |    |
| Xylenes, Total                 | M             | ug/L         | 3.68934    | 0.11227        |                  | 0     | 0        | 0         | 0.0604 | 1      | 0      | 0%   | 0   | 0    | 0%   | J  |
| 1,2-Dichloroethane-d4          | S             | ug/L         | 291.79466  | 11.6717864     |                  | 10    | 0        | 0         | 0.229  | 1      | 500    | 117% | 81  | 118  | 0%   |    |
| Dibromofluoromethane           | S             | ug/L         | 278.83419  | 11.1533676     |                  | 10    | 0        | 0         | 0.129  | 1      | 500    | 112% | 80  | 119  | 0%   |    |
| p-Bromofluorobenzene           | S             | ug/L         | 270.38071  | 10.8152284     |                  | 10    | 0        | 0         | 0.149  | 1      | 500    | 108% | 85  | 114  | 0%   |    |
| Toluene-d8                     | S             | ug/L         | 261.60968  | 10.4643872     |                  | 10    | 0        | 0         | 0.23   | 1      | 500    | 105% | 89  | 112  | 0%   |    |

| Seq No                    | Lab ID        | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|---------------------------|---------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14973463                  | B22010214-001 | VOC-8260-W-S | SAMP       | DA5975CVVG010' | 1/7/2022 3:35:59 | 1     | R373037  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                   | T             | Units        | RAW        | Final          | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.101  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1,1-Trichloroethane     | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.131  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1,2,2-Tetrachloroethane | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0872 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1,2-Trichloroethane     | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.108  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1-Dichloroethane        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.135  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1-Dichloroethene        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.141  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1-Dichloropropene       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.083  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2,3-Trichloropropane    | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.235  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2-Dibromoethane         | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0916 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2-Dichlorobenzene       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0746 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2-Dichloroethane        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.116  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2-Dichloropropane       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0847 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,3-Dichlorobenzene       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0803 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,3-Dichloropropane       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0791 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,4-Dichlorobenzene       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0858 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 2,2-Dichloropropane       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.186  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 2-Chlorotoluene           | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0876 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 4-Chlorotoluene           | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0728 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Benzene                   | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0914 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Bromobenzene              | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0831 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Bromochloromethane        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.141  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Bromodichloromethane      | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.12   | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Bromoform                 | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.119  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Bromomethane              | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.253  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Carbon tetrachloride      | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.143  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Chlorobenzene             | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0914 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Chlorodibromomethane      | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0841 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Chloroethane              | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.169  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Chloroform                | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0789 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Chloromethane             | A             | ug/L         | 1.7362     | 0              |                  | 0     | 0        | 0         | 0.162  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| cis-1,2-Dichloroethene    | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.108  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| cis-1,3-Dichloropropene   | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.073  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Dibromomethane            | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.147  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Dichlorodifluoromethane   | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.175  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Ethylbenzene              | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0836 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |

| Seq No                         | Lab ID        | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |    |
|--------------------------------|---------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|----|
| 14973463                       | B22010214-001 | VOC-8260-W-S | SAMP       | DA5975C\VG010' | 1/7/2022 3:35:59 | 1     | R373037  |           | 0      | 0      |        |      |     |      |      |    |
| Analyte                        | T             | Units        | RAW        | Final          | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q  |
| m+p-Xylenes                    | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.15   | 1      | 1000   | 0%   | 0   | 0    | 0%   | U  |
| Methyl ethyl ketone            | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 1.77   | 20     | 5000   | 0%   | 0   | 0    | 0%   | U  |
| Methyl tert-butyl ether (MTBE) | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.101  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Methylene chloride             | A             | ug/L         | 0.70004    | 0              |                  | 0     | 0        | 0         | 0.338  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| o-Xylene                       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0604 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Styrene                        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.067  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Tetrachloroethene              | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0671 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Toluene                        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0679 | 1      | 500    | 0%   | 0   | 0    | 0%   | UT |
| trans-1,2-Dichloroethene       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.125  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| trans-1,3-Dichloropropene      | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0846 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Trichloroethene                | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0993 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Trichlorofluoromethane         | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.134  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Vinyl chloride                 | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.153  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| 1,4-Dichlorobenzene-d4         | I             | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0      | 0      | 0      | 0%   | 0   | 0    | 0%   |    |
| Chlorobenzene-d5               | I             | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0.1    | 0      | 0      | 0%   | 0   | 0    | 0%   |    |
| Fluorobenzene                  | I             | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0.1    | 0      | 0      | 0%   | 0   | 0    | 0%   |    |
| Xylenes, Total                 | M             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0604 | 1      | 0      | 0%   | 0   | 0    | 0%   | U  |
| 1,2-Dichloroethane-d4          | S             | ug/L         | 287.08913  | 11.4835652     |                  | 10    | 0        | 0         | 0.229  | 1      | 500    | 115% | 81  | 118  | 0%   |    |
| Dibromofluoromethane           | S             | ug/L         | 279.63706  | 11.1854824     |                  | 10    | 0        | 0         | 0.129  | 1      | 500    | 112% | 80  | 119  | 0%   |    |
| p-Bromofluorobenzene           | S             | ug/L         | 276.52735  | 11.061094      |                  | 10    | 0        | 0         | 0.149  | 1      | 500    | 111% | 85  | 114  | 0%   |    |
| Toluene-d8                     | S             | ug/L         | 267.8901   | 10.715604      |                  | 10    | 0        | 0         | 0.23   | 1      | 500    | 107% | 89  | 112  | 0%   |    |

| Seq No                    | Lab ID        | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|---------------------------|---------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14973464                  | B22010262-001 | VOC-8260-W-S | SAMP       | DA5975C\VG010' | 1/7/2022 4:03:14 | 1     | R373037  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                   | T             | Units        | RAW        | Final          | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.101  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1,1-Trichloroethane     | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.131  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1,2,2-Tetrachloroethane | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0872 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1,2-Trichloroethane     | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.108  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1-Dichloroethane        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.135  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1-Dichloroethene        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.141  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1-Dichloropropene       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.083  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2,3-Trichloropropane    | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.235  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2-Dibromoethane         | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0916 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |

| Seq No                         | Lab ID        | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |    |
|--------------------------------|---------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|----|
| 14973464                       | B22010262-001 | VOC-8260-W-S | SAMP       | DA5975C\VG010' | 1/7/2022 4:03:14 | 1     | R373037  |           | 0      | 0      |        |      |     |      |      |    |
| Analyte                        | T             | Units        | RAW        | Final          | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q  |
| 1,2-Dichlorobenzene            | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0746 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| 1,2-Dichloroethane             | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.116  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| 1,2-Dichloropropane            | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0847 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| 1,3-Dichlorobenzene            | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0803 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| 1,3-Dichloropropane            | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0791 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| 1,4-Dichlorobenzene            | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0858 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| 2,2-Dichloropropane            | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.186  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| 2-Chlorotoluene                | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0876 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| 4-Chlorotoluene                | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0728 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Benzene                        | A             | ug/L         | 0.22658    | 0              |                  | 0     | 0        | 0         | 0.0914 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Bromobenzene                   | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0831 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Bromochloromethane             | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.141  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Bromodichloromethane           | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.12   | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Bromoform                      | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.119  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Bromomethane                   | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.253  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Carbon tetrachloride           | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.143  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Chlorobenzene                  | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0914 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Chlorodibromomethane           | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0841 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Chloroethane                   | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.169  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Chloroform                     | A             | ug/L         | 0.38011    | 0              |                  | 0     | 0        | 0         | 0.0789 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Chloromethane                  | A             | ug/L         | 0.4748     | 0              |                  | 0     | 0        | 0         | 0.162  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| cis-1,2-Dichloroethene         | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.108  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| cis-1,3-Dichloropropene        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.073  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Dibromomethane                 | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.147  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Dichlorodifluoromethane        | A             | ug/L         | 1.09038    | 0              |                  | 0     | 0        | 0         | 0.175  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Ethylbenzene                   | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0836 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| m+p-Xylenes                    | A             | ug/L         | 0.33148    | 0              |                  | 0     | 0        | 0         | 0.15   | 1      | 1000   | 0%   | 0   | 0    | 0%   | U  |
| Methyl ethyl ketone            | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 1.77   | 20     | 5000   | 0%   | 0   | 0    | 0%   | U  |
| Methyl tert-butyl ether (MTBE) | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.101  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Methylene chloride             | A             | ug/L         | 0.52611    | 0              |                  | 0     | 0        | 0         | 0.338  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| o-Xylene                       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0604 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Styrene                        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.067  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Tetrachloroethene              | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0671 | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |
| Toluene                        | A             | ug/L         | 0.35025    | 0              |                  | 0     | 0        | 0         | 0.0679 | 1      | 500    | 0%   | 0   | 0    | 0%   | UT |
| trans-1,2-Dichloroethene       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.125  | 1      | 500    | 0%   | 0   | 0    | 0%   | U  |

| Seq No                    | Lab ID        | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|---------------------------|---------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14973464                  | B22010262-001 | VOC-8260-W-S | SAMP       | DA5975C\VG010' | 1/7/2022 4:03:14 | 1     | R373037  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                   | T             | Units        | RAW        | Final          | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| trans-1,3-Dichloropropene | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0846 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Trichloroethene           | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0993 | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Trichlorofluoromethane    | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.134  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| Vinyl chloride            | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.153  | 1      | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,4-Dichlorobenzene-d4    | I             | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0      | 0      | 0      | 0%   | 0   | 0    | 0%   |   |
| Chlorobenzene-d5          | I             | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0.1    | 0      | 0      | 0%   | 0   | 0    | 0%   |   |
| Fluorobenzene             | I             | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0.1    | 0      | 0      | 0%   | 0   | 0    | 0%   |   |
| Xylenes, Total            | M             | ug/L         | 0.33148    | 0              |                  | 0     | 0        | 0         | 0.0604 | 1      | 0      | 0%   | 0   | 0    | 0%   | U |
| 1,2-Dichloroethane-d4     | S             | ug/L         | 286.13131  | 11.4452524     |                  | 10    | 0        | 0         | 0.229  | 1      | 500    | 114% | 81  | 118  | 0%   |   |
| Dibromofluoromethane      | S             | ug/L         | 273.56212  | 10.9424848     |                  | 10    | 0        | 0         | 0.129  | 1      | 500    | 109% | 80  | 119  | 0%   |   |
| p-Bromofluorobenzene      | S             | ug/L         | 269.84089  | 10.7936356     |                  | 10    | 0        | 0         | 0.149  | 1      | 500    | 108% | 85  | 114  | 0%   |   |
| Toluene-d8                | S             | ug/L         | 270.53246  | 10.8212984     |                  | 10    | 0        | 0         | 0.23   | 1      | 500    | 108% | 89  | 112  | 0%   |   |

| Seq No                    | Lab ID        | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|---------------------------|---------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14973525                  | B22010219-001 | VOC-8260-W-Q | SAMP       | DA5975C\VG010' | 1/7/2022 2:14:04 | 1     | R373037  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                   | T             | Units        | RAW        | Final          | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.101  | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1,1-Trichloroethane     | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.131  | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1,2,2-Tetrachloroethane | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0872 | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1,2-Trichloroethane     | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.108  | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1-Dichloroethane        | A             | ug/L         | 0.6175     | 0              |                  | 0     | 0        | 0         | 0.135  | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1-Dichloroethene        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.141  | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,1-Dichloropropene       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.083  | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2,3-Trichloropropane    | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.235  | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2-Dibromoethane         | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0916 | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2-Dichlorobenzene       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0746 | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2-Dichloroethane        | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.116  | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,2-Dichloropropane       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0847 | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,3-Dichlorobenzene       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0803 | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,3-Dichloropropane       | A             | ug/L         | 0.40048    | 0              |                  | 0     | 0        | 0         | 0.0791 | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,4-Dichlorobenzene       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0858 | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| 2,2-Dichloropropane       | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.186  | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| 2-Chlorotoluene           | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0876 | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| 4-Chlorotoluene           | A             | ug/L         | 0          | 0              |                  | 0     | 0        | 0         | 0.0728 | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |

| Seq No                         | Lab ID        | Test Code    | Sample Typ | File ID       | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|--------------------------------|---------------|--------------|------------|---------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14973525                       | B22010219-001 | VOC-8260-W-Q | SAMP       | DA5975CVVG010 | 1/7/2022 2:14:04 | 1     | R373037  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                        | T             | Units        | RAW        | Final         | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| Benzene                        | A             | ug/L         | 0.43706    | 0             |                  | 0     | 0        | 0         | 0.0914 | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| Bromobenzene                   | A             | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0831 | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| Bromochloromethane             | A             | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.141  | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| Bromodichloromethane           | A             | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.12   | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| Bromoform                      | A             | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.119  | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| Bromomethane                   | A             | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.253  | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| Carbon tetrachloride           | A             | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.143  | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| Chlorobenzene                  | A             | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0914 | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| Chlorodibromomethane           | A             | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0841 | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| Chloroethane                   | A             | ug/L         | 2.80665    | 0             |                  | 0     | 0        | 0         | 0.169  | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| Chloroform                     | A             | ug/L         | 0.50573    | 0             |                  | 0     | 0        | 0         | 0.0789 | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| Chloromethane                  | A             | ug/L         | 1.01509    | 0             |                  | 0     | 0        | 0         | 0.162  | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| cis-1,2-Dichloroethene         | A             | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.108  | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| cis-1,3-Dichloropropene        | A             | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.073  | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| Dibromomethane                 | A             | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.147  | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| Dichlorodifluoromethane        | A             | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.175  | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| Ethylbenzene                   | A             | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0836 | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| m+p-Xylenes                    | A             | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.15   | 0.5    | 1000   | 0%   | 0   | 0    | 0%   | U |
| Methyl ethyl ketone            | A             | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 1.77   | 10     | 5000   | 0%   | 0   | 0    | 0%   | U |
| Methyl tert-butyl ether (MTBE) | A             | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.101  | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| Methylene chloride             | A             | ug/L         | 1.07273    | 0             |                  | 0     | 0        | 0         | 0.338  | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| o-Xylene                       | A             | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0604 | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| Styrene                        | A             | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.067  | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| Tetrachloroethene              | A             | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0671 | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| Toluene                        | A             | ug/L         | 0.34358    | 0             |                  | 0     | 0        | 0         | 0.0679 | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| trans-1,2-Dichloroethene       | A             | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.125  | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| trans-1,3-Dichloropropene      | A             | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0846 | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| Trichloroethene                | A             | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0993 | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| Trichlorofluoromethane         | A             | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.134  | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| Vinyl chloride                 | A             | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.153  | 0.5    | 500    | 0%   | 0   | 0    | 0%   | U |
| 1,4-Dichlorobenzene-d4         | I             | ug/L         | 250        | 10            |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 0   | 0    | 0%   |   |
| Chlorobenzene-d5               | I             | ug/L         | 250        | 10            |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 0   | 0    | 0%   |   |
| Fluorobenzene                  | I             | ug/L         | 250        | 10            |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 0   | 0    | 0%   |   |
| Xylenes, Total                 | M             | ug/L         | 0          | 0             |                  | 0     | 0        | 0         | 0.0604 | 0.5    | 1500   | 0%   | 0   | 0    | 0%   | U |
| 1,2-Dichloroethane-d4          | S             | ug/L         | 295.01742  | 11.8006968    |                  | 10    | 0        | 0         | 0.229  | 0.5    | 500    | 118% | 81  | 118  | 0%   |   |

| Seq No               | Lab ID        | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|----------------------|---------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14973525             | B22010219-001 | VOC-8260-W-Q | SAMP       | DA5975C\VG010' | 1/7/2022 2:14:04 | 1     | R373037  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte              | T             | Units        | RAW        | Final          | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| Dibromofluoromethane | S             | ug/L         | 277.84253  | 11.1137012     |                  | 10    | 0        | 0         | 0.129  | 0.5    | 500    | 111% | 80  | 119  | 0%   |   |
| p-Bromofluorobenzene | S             | ug/L         | 270.69927  | 10.8279708     |                  | 10    | 0        | 0         | 0.149  | 0.5    | 500    | 108% | 85  | 114  | 0%   |   |
| Toluene-d8           | S             | ug/L         | 269.72701  | 10.7890804     |                  | 10    | 0        | 0         | 0.23   | 0.5    | 500    | 108% | 89  | 112  | 0%   |   |

| Seq No                    | Lab ID        | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|---------------------------|---------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14973526                  | B22010219-001 | VOC-8260-W-Q | MS-DOD     | DA5975C\VG010' | 1/7/2022 5:07:38 | 1     | R373037  |           | 1E+07  | 0      |        |      |     |      |      |   |
| Analyte                   | T             | Units        | RAW        | Final          | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A             | ug/L         | 123.97204  | 4.9588816      |                  | 5     | 0        | 0         | 0.101  | 0.5    | 500    | 99%  | 78  | 124  | 0%   |   |
| 1,1,1-Trichloroethane     | A             | ug/L         | 124.76854  | 4.9907416      |                  | 5     | 0        | 0         | 0.131  | 0.5    | 500    | 100% | 74  | 131  | 0%   |   |
| 1,1,2,2-Tetrachloroethane | A             | ug/L         | 131.23289  | 5.2493156      |                  | 5     | 0        | 0         | 0.0872 | 0.5    | 500    | 105% | 71  | 121  | 0%   |   |
| 1,1,2-Trichloroethane     | A             | ug/L         | 123.55913  | 4.9423652      |                  | 5     | 0        | 0         | 0.108  | 0.5    | 500    | 99%  | 80  | 119  | 0%   |   |
| 1,1-Dichloroethane        | A             | ug/L         | 135.5713   | 5.422852       |                  | 5     | 0        | 0         | 0.135  | 0.5    | 500    | 108% | 77  | 125  | 0%   |   |
| 1,1-Dichloroethene        | A             | ug/L         | 131.07964  | 5.2431856      |                  | 5     | 0        | 0         | 0.141  | 0.5    | 500    | 105% | 71  | 131  | 0%   |   |
| 1,1-Dichloropropene       | A             | ug/L         | 121.41514  | 4.8566056      |                  | 5     | 0        | 0         | 0.083  | 0.5    | 500    | 97%  | 79  | 125  | 0%   |   |
| 1,2,3-Trichloropropane    | A             | ug/L         | 123.82462  | 4.9529848      |                  | 5     | 0        | 0         | 0.235  | 0.5    | 500    | 99%  | 73  | 125  | 0%   |   |
| 1,2-Dibromoethane         | A             | ug/L         | 124.83894  | 4.9935576      |                  | 5     | 0        | 0         | 0.0916 | 0.5    | 500    | 100% | 78  | 122  | 0%   |   |
| 1,2-Dichlorobenzene       | A             | ug/L         | 125.95905  | 5.038362       |                  | 5     | 0        | 0         | 0.0746 | 0.5    | 500    | 101% | 80  | 119  | 0%   |   |
| 1,2-Dichloroethane        | A             | ug/L         | 127.86267  | 5.1145068      |                  | 5     | 0        | 0         | 0.116  | 0.5    | 500    | 102% | 73  | 128  | 0%   |   |
| 1,2-Dichloropropane       | A             | ug/L         | 125.3364   | 5.013456       |                  | 5     | 0        | 0         | 0.0847 | 0.5    | 500    | 100% | 78  | 122  | 0%   |   |
| 1,3-Dichlorobenzene       | A             | ug/L         | 131.39699  | 5.2558796      |                  | 5     | 0        | 0         | 0.0803 | 0.5    | 500    | 105% | 80  | 119  | 0%   |   |
| 1,3-Dichloropropane       | A             | ug/L         | 126.75683  | 5.0702732      |                  | 5     | 0        | 0         | 0.0791 | 0.5    | 500    | 101% | 80  | 119  | 0%   |   |
| 1,4-Dichlorobenzene       | A             | ug/L         | 129.89641  | 5.1958564      |                  | 5     | 0        | 0         | 0.0858 | 0.5    | 500    | 104% | 79  | 118  | 0%   |   |
| 2,2-Dichloropropane       | A             | ug/L         | 131.81307  | 5.2725228      |                  | 5     | 0        | 0         | 0.186  | 0.5    | 500    | 105% | 60  | 139  | 0%   |   |
| 2-Chlorotoluene           | A             | ug/L         | 131.31335  | 5.252534       |                  | 5     | 0        | 0         | 0.0876 | 0.5    | 500    | 105% | 79  | 122  | 0%   |   |
| 4-Chlorotoluene           | A             | ug/L         | 133.3048   | 5.332192       |                  | 5     | 0        | 0         | 0.0728 | 0.5    | 500    | 107% | 78  | 122  | 0%   |   |
| Benzene                   | A             | ug/L         | 130.23088  | 5.2092352      |                  | 5     | 0        | 0         | 0.0914 | 0.5    | 500    | 104% | 79  | 120  | 0%   |   |
| Bromobenzene              | A             | ug/L         | 133.61494  | 5.3445976      |                  | 5     | 0        | 0         | 0.0831 | 0.5    | 500    | 107% | 80  | 120  | 0%   |   |
| Bromochloromethane        | A             | ug/L         | 124.44772  | 4.9779088      |                  | 5     | 0        | 0         | 0.141  | 0.5    | 500    | 100% | 78  | 123  | 0%   |   |
| Bromodichloromethane      | A             | ug/L         | 128.24178  | 5.1296712      |                  | 5     | 0        | 0         | 0.12   | 0.5    | 500    | 103% | 79  | 125  | 0%   |   |
| Bromoform                 | A             | ug/L         | 129.70364  | 5.1881456      |                  | 5     | 0        | 0         | 0.119  | 0.5    | 500    | 104% | 66  | 130  | 0%   |   |
| Bromomethane              | A             | ug/L         | 120.98596  | 4.8394384      |                  | 5     | 0        | 0         | 0.253  | 0.5    | 500    | 97%  | 53  | 141  | 0%   |   |
| Carbon tetrachloride      | A             | ug/L         | 121.69468  | 4.8677872      |                  | 5     | 0        | 0         | 0.143  | 0.5    | 500    | 97%  | 72  | 136  | 0%   |   |
| Chlorobenzene             | A             | ug/L         | 128.27202  | 5.1308808      |                  | 5     | 0        | 0         | 0.0914 | 0.5    | 500    | 103% | 82  | 118  | 0%   |   |
| Chlorodibromomethane      | A             | ug/L         | 125.15946  | 5.0063784      |                  | 5     | 0        | 0         | 0.0841 | 0.5    | 500    | 100% | 74  | 126  | 0%   |   |

| Seq No                         | Lab ID        | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|--------------------------------|---------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14973526                       | B22010219-001 | VOC-8260-W-Q | MS-DOD     | DA5975C\VG010' | 1/7/2022 5:07:38 | 1     | R373037  |           | 1E+07  | 0      |        |      |     |      |      |   |
| Analyte                        | T             | Units        | RAW        | Final          | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| Chloroethane                   | A             | ug/L         | 141.01823  | 5.6407292      |                  | 5     | 0        | 0         | 0.169  | 0.5    | 500    | 113% | 60  | 138  | 0%   |   |
| Chloroform                     | A             | ug/L         | 121.47415  | 4.858966       |                  | 5     | 0        | 0         | 0.0789 | 0.5    | 500    | 97%  | 79  | 124  | 0%   |   |
| Chloromethane                  | A             | ug/L         | 111.80488  | 4.4721952      |                  | 5     | 0        | 0         | 0.162  | 0.5    | 500    | 89%  | 50  | 139  | 0%   |   |
| cis-1,2-Dichloroethene         | A             | ug/L         | 131.27992  | 5.2511968      |                  | 5     | 0        | 0         | 0.108  | 0.5    | 500    | 105% | 78  | 123  | 0%   |   |
| cis-1,3-Dichloropropene        | A             | ug/L         | 121.0494   | 4.841976       |                  | 5     | 0        | 0         | 0.073  | 0.5    | 500    | 97%  | 75  | 124  | 0%   |   |
| Dibromomethane                 | A             | ug/L         | 125.77977  | 5.0311908      |                  | 5     | 0        | 0         | 0.147  | 0.5    | 500    | 101% | 79  | 123  | 0%   |   |
| Dichlorodifluoromethane        | A             | ug/L         | 107.33342  | 4.2933368      |                  | 5     | 0        | 0         | 0.175  | 0.5    | 500    | 86%  | 32  | 152  | 0%   |   |
| Ethylbenzene                   | A             | ug/L         | 127.05741  | 5.0822964      |                  | 5     | 0        | 0         | 0.0836 | 0.5    | 500    | 102% | 79  | 121  | 0%   |   |
| m+p-Xylenes                    | A             | ug/L         | 253.24827  | 10.1299308     |                  | 10    | 0        | 0         | 0.15   | 0.5    | 1000   | 101% | 80  | 121  | 0%   |   |
| Methyl ethyl ketone            | A             | ug/L         | 1256.63414 | 50.2653656     |                  | 50    | 0        | 0         | 1.77   | 10     | 5000   | 101% | 56  | 143  | 0%   |   |
| Methyl tert-butyl ether (MTBE) | A             | ug/L         | 140.12523  | 5.6050092      |                  | 5     | 0        | 0         | 0.101  | 0.5    | 500    | 112% | 71  | 124  | 0%   |   |
| Methylene chloride             | A             | ug/L         | 121.94927  | 4.8779708      |                  | 5     | 0        | 0         | 0.338  | 0.5    | 500    | 98%  | 74  | 124  | 0%   |   |
| o-Xylene                       | A             | ug/L         | 130.73381  | 5.2293524      |                  | 5     | 0        | 0         | 0.0604 | 0.5    | 500    | 105% | 78  | 122  | 0%   |   |
| Styrene                        | A             | ug/L         | 132.42019  | 5.2968076      |                  | 5     | 0        | 0         | 0.067  | 0.5    | 500    | 106% | 78  | 123  | 0%   |   |
| Tetrachloroethene              | A             | ug/L         | 122.39033  | 4.8956132      |                  | 5     | 0        | 0         | 0.0671 | 0.5    | 500    | 98%  | 74  | 129  | 0%   |   |
| Toluene                        | A             | ug/L         | 129.27156  | 5.1708624      |                  | 5     | 0        | 0         | 0.0679 | 0.5    | 500    | 103% | 80  | 121  | 0%   |   |
| trans-1,2-Dichloroethene       | A             | ug/L         | 129.83227  | 5.1932908      |                  | 5     | 0        | 0         | 0.125  | 0.5    | 500    | 104% | 75  | 124  | 0%   |   |
| trans-1,3-Dichloropropene      | A             | ug/L         | 132.48323  | 5.2993292      |                  | 5     | 0        | 0         | 0.0846 | 0.5    | 500    | 106% | 73  | 127  | 0%   |   |
| Trichloroethene                | A             | ug/L         | 125.4471   | 5.017884       |                  | 5     | 0        | 0         | 0.0993 | 0.5    | 500    | 100% | 79  | 123  | 0%   |   |
| Trichlorofluoromethane         | A             | ug/L         | 124.51499  | 4.9805996      |                  | 5     | 0        | 0         | 0.134  | 0.5    | 500    | 100% | 65  | 141  | 0%   |   |
| Vinyl chloride                 | A             | ug/L         | 122.60319  | 4.9041276      |                  | 5     | 0        | 0         | 0.153  | 0.5    | 500    | 98%  | 58  | 137  | 0%   |   |
| 1,4-Dichlorobenzene-d4         | I             | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 0   | 0    | 0%   |   |
| Chlorobenzene-d5               | I             | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 0   | 0    | 0%   |   |
| Fluorobenzene                  | I             | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 0   | 0    | 0%   |   |
| Xylenes, Total                 | M             | ug/L         | 383.98208  | 15.3592832     |                  | 15    | 0        | 0         | 0.0604 | 0.5    | 1500   | 102% | 79  | 121  | 0%   |   |
| 1,2-Dichloroethane-d4          | S             | ug/L         | 277.78361  | 11.1113444     |                  | 10    | 0        | 0         | 0.229  | 0.5    | 500    | 111% | 81  | 118  | 0%   |   |
| Dibromofluoromethane           | S             | ug/L         | 273.52362  | 10.9409448     |                  | 10    | 0        | 0         | 0.129  | 0.5    | 500    | 109% | 80  | 119  | 0%   |   |
| p-Bromofluorobenzene           | S             | ug/L         | 274.05376  | 10.9621504     |                  | 10    | 0        | 0         | 0.149  | 0.5    | 500    | 110% | 85  | 114  | 0%   |   |
| Toluene-d8                     | S             | ug/L         | 271.7626   | 10.870504      |                  | 10    | 0        | 0         | 0.23   | 0.5    | 500    | 109% | 89  | 112  | 0%   |   |

| Seq No   | Lab ID        | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|----------|---------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14973527 | B22010219-001 | VOC-8260-W-Q | MSD-DOD    | DA5975C\VG010' | 1/7/2022 5:34:50 | 1     | R373037  |           | 1E+07  | 1E+07  |        |      |     |      |      |   |
| Analyte  | T             | Units        | RAW        | Final          | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |



| Seq No                    | Lab ID        | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID    | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|---------------------------|---------------|--------------|------------|----------------|------------------|-------|-------------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14973527                  | B22010219-001 | VOC-8260-W-Q | MSD-DOD    | DA5975C\VG010' | 1/7/2022 5:34:50 | 1     | R373037     |           | 1E+07  | 1E+07  |        |      |     |      |      |   |
| Analyte                   | T             | Units        | RAW        | Final          | Text             | Spike | SPKref      | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A             | ug/L         | 126.97081  | 5.0788324      |                  | 5     | 0 4.9588816 | 0.101     | 0.5    | 500    | 102%   | 78   | 124 | 2%   |      |   |
| 1,1,1-Trichloroethane     | A             | ug/L         | 129.67471  | 5.1869884      |                  | 5     | 0 4.9907416 | 0.131     | 0.5    | 500    | 104%   | 74   | 131 | 4%   |      |   |
| 1,1,2,2-Tetrachloroethane | A             | ug/L         | 137.05211  | 5.4820844      |                  | 5     | 0 5.2493156 | 0.0872    | 0.5    | 500    | 110%   | 71   | 121 | 4%   |      |   |
| 1,1,2-Trichloroethane     | A             | ug/L         | 128.35043  | 5.1340172      |                  | 5     | 0 4.9423652 | 0.108     | 0.5    | 500    | 103%   | 80   | 119 | 4%   |      |   |
| 1,1-Dichloroethane        | A             | ug/L         | 139.44565  | 5.577826       |                  | 5     | 0 5.422852  | 0.135     | 0.5    | 500    | 112%   | 77   | 125 | 3%   |      |   |
| 1,1-Dichloroethene        | A             | ug/L         | 134.54038  | 5.3816152      |                  | 5     | 0 5.2431856 | 0.141     | 0.5    | 500    | 108%   | 71   | 131 | 3%   |      |   |
| 1,1-Dichloropropene       | A             | ug/L         | 125.60877  | 5.0243508      |                  | 5     | 0 4.8566056 | 0.083     | 0.5    | 500    | 100%   | 79   | 125 | 3%   |      |   |
| 1,2,3-Trichloropropane    | A             | ug/L         | 134.57211  | 5.3828844      |                  | 5     | 0 4.9529848 | 0.235     | 0.5    | 500    | 108%   | 73   | 125 | 8%   |      |   |
| 1,2-Dibromoethane         | A             | ug/L         | 131.63801  | 5.2655204      |                  | 5     | 0 4.9935576 | 0.0916    | 0.5    | 500    | 105%   | 78   | 122 | 5%   |      |   |
| 1,2-Dichlorobenzene       | A             | ug/L         | 132.96807  | 5.3187228      |                  | 5     | 0 5.038362  | 0.0746    | 0.5    | 500    | 106%   | 80   | 119 | 5%   |      |   |
| 1,2-Dichloroethane        | A             | ug/L         | 127.77295  | 5.110918       |                  | 5     | 0 5.1145068 | 0.116     | 0.5    | 500    | 102%   | 73   | 128 | 0%   |      |   |
| 1,2-Dichloropropane       | A             | ug/L         | 133.30768  | 5.3323072      |                  | 5     | 0 5.013456  | 0.0847    | 0.5    | 500    | 107%   | 78   | 122 | 6%   |      |   |
| 1,3-Dichlorobenzene       | A             | ug/L         | 137.9499   | 5.517996       |                  | 5     | 0 5.2558796 | 0.0803    | 0.5    | 500    | 110%   | 80   | 119 | 5%   |      |   |
| 1,3-Dichloropropane       | A             | ug/L         | 132.70403  | 5.3081612      |                  | 5     | 0 5.0702732 | 0.0791    | 0.5    | 500    | 106%   | 80   | 119 | 5%   |      |   |
| 1,4-Dichlorobenzene       | A             | ug/L         | 137.42865  | 5.497146       |                  | 5     | 0 5.1958564 | 0.0858    | 0.5    | 500    | 110%   | 79   | 118 | 6%   |      |   |
| 2,2-Dichloropropane       | A             | ug/L         | 141.24186  | 5.6496744      |                  | 5     | 0 5.2725228 | 0.186     | 0.5    | 500    | 113%   | 60   | 139 | 7%   |      |   |
| 2-Chlorotoluene           | A             | ug/L         | 141.2126   | 5.648504       |                  | 5     | 0 5.252534  | 0.0876    | 0.5    | 500    | 113%   | 79   | 122 | 7%   |      |   |
| 4-Chlorotoluene           | A             | ug/L         | 142.04727  | 5.6818908      |                  | 5     | 0 5.332192  | 0.0728    | 0.5    | 500    | 114%   | 78   | 122 | 6%   |      |   |
| Benzene                   | A             | ug/L         | 133.07465  | 5.322986       |                  | 5     | 0 5.2092352 | 0.0914    | 0.5    | 500    | 106%   | 79   | 120 | 2%   |      |   |
| Bromobenzene              | A             | ug/L         | 142.54012  | 5.7016048      |                  | 5     | 0 5.3445976 | 0.0831    | 0.5    | 500    | 114%   | 80   | 120 | 6%   |      |   |
| Bromochloromethane        | A             | ug/L         | 127.87548  | 5.1150192      |                  | 5     | 0 4.9779088 | 0.141     | 0.5    | 500    | 102%   | 78   | 123 | 3%   |      |   |
| Bromodichloromethane      | A             | ug/L         | 135.38706  | 5.4154824      |                  | 5     | 0 5.1296712 | 0.12      | 0.5    | 500    | 108%   | 79   | 125 | 5%   |      |   |
| Bromoform                 | A             | ug/L         | 139.78015  | 5.591206       |                  | 5     | 0 5.1881456 | 0.119     | 0.5    | 500    | 112%   | 66   | 130 | 7%   |      |   |
| Bromomethane              | A             | ug/L         | 119.87937  | 4.7951748      |                  | 5     | 0 4.8394384 | 0.253     | 0.5    | 500    | 96%    | 53   | 141 | 1%   |      |   |
| Carbon tetrachloride      | A             | ug/L         | 124.65019  | 4.9860076      |                  | 5     | 0 4.8677872 | 0.143     | 0.5    | 500    | 100%   | 72   | 136 | 2%   |      |   |
| Chlorobenzene             | A             | ug/L         | 135.94651  | 5.4378604      |                  | 5     | 0 5.1308808 | 0.0914    | 0.5    | 500    | 109%   | 82   | 118 | 6%   |      |   |
| Chlorodibromomethane      | A             | ug/L         | 127.72526  | 5.1090104      |                  | 5     | 0 5.0063784 | 0.0841    | 0.5    | 500    | 102%   | 74   | 126 | 2%   |      |   |
| Chloroethane              | A             | ug/L         | 121.58436  | 4.8633744      |                  | 5     | 0 5.6407292 | 0.169     | 0.5    | 500    | 97%    | 60   | 138 | 15%  |      |   |
| Chloroform                | A             | ug/L         | 126.24502  | 5.0498008      |                  | 5     | 0 4.858966  | 0.0789    | 0.5    | 500    | 101%   | 79   | 124 | 4%   |      |   |
| Chloromethane             | A             | ug/L         | 117.71804  | 4.7087216      |                  | 5     | 0 4.4721952 | 0.162     | 0.5    | 500    | 94%    | 50   | 139 | 5%   |      |   |
| cis-1,2-Dichloroethene    | A             | ug/L         | 133.90986  | 5.3563944      |                  | 5     | 0 5.2511968 | 0.108     | 0.5    | 500    | 107%   | 78   | 123 | 2%   |      |   |
| cis-1,3-Dichloropropene   | A             | ug/L         | 127.54766  | 5.1019064      |                  | 5     | 0 4.841976  | 0.073     | 0.5    | 500    | 102%   | 75   | 124 | 5%   |      |   |
| Dibromomethane            | A             | ug/L         | 129.42028  | 5.1768112      |                  | 5     | 0 5.0311908 | 0.147     | 0.5    | 500    | 104%   | 79   | 123 | 3%   |      |   |
| Dichlorodifluoromethane   | A             | ug/L         | 110.63166  | 4.4252664      |                  | 5     | 0 4.2933368 | 0.175     | 0.5    | 500    | 89%    | 32   | 152 | 3%   |      |   |
| Ethylbenzene              | A             | ug/L         | 135.43417  | 5.4173668      |                  | 5     | 0 5.0822964 | 0.0836    | 0.5    | 500    | 108%   | 79   | 121 | 6%   |      |   |

| Seq No                         | Lab ID        | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|--------------------------------|---------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14973527                       | B22010219-001 | VOC-8260-W-Q | MSD-DOD    | DA5975C\VG010' | 1/7/2022 5:34:50 | 1     | R373037  |           | 1E+07  | 1E+07  |        |      |     |      |      |   |
| Analyte                        | T             | Units        | RAW        | Final          | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| m+p-Xylenes                    | A             | ug/L         | 265.23121  | 10.6092484     |                  | 10    | 0        | 10.129931 | 0.15   | 0.5    | 1000   | 106% | 80  | 121  | 5%   |   |
| Methyl ethyl ketone            | A             | ug/L         | 1218.10205 | 48.724082      |                  | 50    | 0        | 50.265366 | 1.77   | 10     | 5000   | 97%  | 56  | 143  | 3%   |   |
| Methyl tert-butyl ether (MTBE) | A             | ug/L         | 142.97082  | 5.7188328      |                  | 5     | 0        | 5.6050092 | 0.101  | 0.5    | 500    | 114% | 71  | 124  | 2%   |   |
| Methylene chloride             | A             | ug/L         | 125.73719  | 5.0294876      |                  | 5     | 0        | 4.8779708 | 0.338  | 0.5    | 500    | 101% | 74  | 124  | 3%   |   |
| o-Xylene                       | A             | ug/L         | 139.35978  | 5.5743912      |                  | 5     | 0        | 5.2293524 | 0.0604 | 0.5    | 500    | 111% | 78  | 122  | 6%   |   |
| Styrene                        | A             | ug/L         | 141.51056  | 5.6604224      |                  | 5     | 0        | 5.2968076 | 0.067  | 0.5    | 500    | 113% | 78  | 123  | 7%   |   |
| Tetrachloroethene              | A             | ug/L         | 132.08546  | 5.2834184      |                  | 5     | 0        | 4.8956132 | 0.0671 | 0.5    | 500    | 106% | 74  | 129  | 8%   |   |
| Toluene                        | A             | ug/L         | 138.2772   | 5.531088       |                  | 5     | 0        | 5.1708624 | 0.0679 | 0.5    | 500    | 111% | 80  | 121  | 7%   |   |
| trans-1,2-Dichloroethene       | A             | ug/L         | 138.08523  | 5.5234092      |                  | 5     | 0        | 5.1932908 | 0.125  | 0.5    | 500    | 110% | 75  | 124  | 6%   |   |
| trans-1,3-Dichloropropene      | A             | ug/L         | 135.69869  | 5.4279476      |                  | 5     | 0        | 5.2993292 | 0.0846 | 0.5    | 500    | 109% | 73  | 127  | 2%   |   |
| Trichloroethene                | A             | ug/L         | 133.54359  | 5.3417436      |                  | 5     | 0        | 5.017884  | 0.0993 | 0.5    | 500    | 107% | 79  | 123  | 6%   |   |
| Trichlorofluoromethane         | A             | ug/L         | 120.34118  | 4.8136472      |                  | 5     | 0        | 4.9805996 | 0.134  | 0.5    | 500    | 96%  | 65  | 141  | 3%   |   |
| Vinyl chloride                 | A             | ug/L         | 125.03335  | 5.001334       |                  | 5     | 0        | 4.9041276 | 0.153  | 0.5    | 500    | 100% | 58  | 137  | 2%   |   |
| 1,4-Dichlorobenzene-d4         | I             | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 0   | 0    | 0%   |   |
| Chlorobenzene-d5               | I             | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 0   | 0    | 0%   |   |
| Fluorobenzene                  | I             | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 0   | 0    | 0%   |   |
| Xylenes, Total                 | M             | ug/L         | 404.59099  | 16.1836396     |                  | 15    | 0        | 15.359283 | 0.0604 | 0.5    | 1500   | 108% | 79  | 121  | 5%   |   |
| 1,2-Dichloroethane-d4          | S             | ug/L         | 272.54518  | 10.9018072     |                  | 10    | 0        | 0         | 0.229  | 0.5    | 500    | 109% | 81  | 118  | 0%   |   |
| Dibromofluoromethane           | S             | ug/L         | 268.6027   | 10.744108      |                  | 10    | 0        | 0         | 0.129  | 0.5    | 500    | 107% | 80  | 119  | 0%   |   |
| p-Bromofluorobenzene           | S             | ug/L         | 271.17267  | 10.8469068     |                  | 10    | 0        | 0         | 0.149  | 0.5    | 500    | 108% | 85  | 114  | 0%   |   |
| Toluene-d8                     | S             | ug/L         | 276.39197  | 11.0556788     |                  | 10    | 0        | 0         | 0.23   | 0.5    | 500    | 111% | 89  | 112  | 0%   |   |

| Seq No                    | Lab ID       | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|---------------------------|--------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14973528                  | CCV010722_CI | VOC-8260-W-Q | CCV        | DA5975C\VG010' | 1/7/2022 6:29:09 | 1     | R373037  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                   | T            | Units        | RAW        | Final          | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| 1,1,1,2-Tetrachloroethane | A            | ug/L         | 116.51857  | 4.6607428      |                  | 5     | 0        | 0         | 0.101  | 0.5    | 500    | 93%  | 50  | 150  | 0%   |   |
| 1,1,1-Trichloroethane     | A            | ug/L         | 118.9139   | 4.756556       |                  | 5     | 0        | 0         | 0.131  | 0.5    | 500    | 95%  | 50  | 150  | 0%   |   |
| 1,1,2,2-Tetrachloroethane | A            | ug/L         | 121.30049  | 4.8520196      |                  | 5     | 0        | 0         | 0.0872 | 0.5    | 500    | 97%  | 50  | 150  | 0%   |   |
| 1,1,2-Trichloroethane     | A            | ug/L         | 116.98429  | 4.6793716      |                  | 5     | 0        | 0         | 0.108  | 0.5    | 500    | 94%  | 50  | 150  | 0%   |   |
| 1,1-Dichloroethane        | A            | ug/L         | 125.05691  | 5.0022764      |                  | 5     | 0        | 0         | 0.135  | 0.5    | 500    | 100% | 50  | 150  | 0%   |   |
| 1,1-Dichloroethene        | A            | ug/L         | 118.78652  | 4.7514608      |                  | 5     | 0        | 0         | 0.141  | 0.5    | 500    | 95%  | 50  | 150  | 0%   |   |
| 1,1-Dichloropropene       | A            | ug/L         | 119.866    | 4.79464        |                  | 5     | 0        | 0         | 0.083  | 0.5    | 500    | 96%  | 50  | 150  | 0%   |   |
| 1,2,3-Trichloropropane    | A            | ug/L         | 114.97648  | 4.5990592      |                  | 5     | 0        | 0         | 0.235  | 0.5    | 500    | 92%  | 50  | 150  | 0%   |   |
| 1,2-Dibromoethane         | A            | ug/L         | 120.00893  | 4.8003572      |                  | 5     | 0        | 0         | 0.0916 | 0.5    | 500    | 96%  | 50  | 150  | 0%   |   |

| Seq No                         | Lab ID       | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|--------------------------------|--------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14973528                       | CCV010722_CI | VOC-8260-W-Q | CCV        | DA5975CVVG010' | 1/7/2022 6:29:09 | 1     | R373037  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                        | T            | Units        | RAW        | Final          | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| 1,2-Dichlorobenzene            | A            | ug/L         | 118.73276  | 4.7493104      |                  | 5     | 0        | 0         | 0.0746 | 0.5    | 500    | 95%  | 50  | 150  | 0%   |   |
| 1,2-Dichloroethane             | A            | ug/L         | 115.09774  | 4.6039096      |                  | 5     | 0        | 0         | 0.116  | 0.5    | 500    | 92%  | 50  | 150  | 0%   |   |
| 1,2-Dichloropropane            | A            | ug/L         | 123.78967  | 4.9515868      |                  | 5     | 0        | 0         | 0.0847 | 0.5    | 500    | 99%  | 50  | 150  | 0%   |   |
| 1,3-Dichlorobenzene            | A            | ug/L         | 121.39871  | 4.8559484      |                  | 5     | 0        | 0         | 0.0803 | 0.5    | 500    | 97%  | 50  | 150  | 0%   |   |
| 1,3-Dichloropropane            | A            | ug/L         | 121.54909  | 4.8619636      |                  | 5     | 0        | 0         | 0.0791 | 0.5    | 500    | 97%  | 50  | 150  | 0%   |   |
| 1,4-Dichlorobenzene            | A            | ug/L         | 120.7629   | 4.830516       |                  | 5     | 0        | 0         | 0.0858 | 0.5    | 500    | 97%  | 50  | 150  | 0%   |   |
| 2,2-Dichloropropane            | A            | ug/L         | 121.75209  | 4.8700836      |                  | 5     | 0        | 0         | 0.186  | 0.5    | 500    | 97%  | 50  | 150  | 0%   |   |
| 2-Chlorotoluene                | A            | ug/L         | 123.99093  | 4.9596372      |                  | 5     | 0        | 0         | 0.0876 | 0.5    | 500    | 99%  | 50  | 150  | 0%   |   |
| 4-Chlorotoluene                | A            | ug/L         | 126.3413   | 5.053652       |                  | 5     | 0        | 0         | 0.0728 | 0.5    | 500    | 101% | 50  | 150  | 0%   |   |
| Benzene                        | A            | ug/L         | 122.52703  | 4.9010812      |                  | 5     | 0        | 0         | 0.0914 | 0.5    | 500    | 98%  | 50  | 150  | 0%   |   |
| Bromobenzene                   | A            | ug/L         | 124.73788  | 4.9895152      |                  | 5     | 0        | 0         | 0.0831 | 0.5    | 500    | 100% | 50  | 150  | 0%   |   |
| Bromochloromethane             | A            | ug/L         | 115.32869  | 4.6131476      |                  | 5     | 0        | 0         | 0.141  | 0.5    | 500    | 92%  | 50  | 150  | 0%   |   |
| Bromodichloromethane           | A            | ug/L         | 118.25683  | 4.7302732      |                  | 5     | 0        | 0         | 0.12   | 0.5    | 500    | 95%  | 50  | 150  | 0%   |   |
| Bromoform                      | A            | ug/L         | 120.83294  | 4.8333176      |                  | 5     | 0        | 0         | 0.119  | 0.5    | 500    | 97%  | 50  | 150  | 0%   |   |
| Bromomethane                   | A            | ug/L         | 124.27001  | 4.9708004      |                  | 5     | 0        | 0         | 0.253  | 0.5    | 500    | 99%  | 50  | 150  | 0%   |   |
| Carbon tetrachloride           | A            | ug/L         | 117.6182   | 4.704728       |                  | 5     | 0        | 0         | 0.143  | 0.5    | 500    | 94%  | 50  | 150  | 0%   |   |
| Chlorobenzene                  | A            | ug/L         | 121.07577  | 4.8430308      |                  | 5     | 0        | 0         | 0.0914 | 0.5    | 500    | 97%  | 50  | 150  | 0%   |   |
| Chlorodibromomethane           | A            | ug/L         | 118.19991  | 4.7279964      |                  | 5     | 0        | 0         | 0.0841 | 0.5    | 500    | 95%  | 50  | 150  | 0%   |   |
| Chloroethane                   | A            | ug/L         | 121.35074  | 4.8540296      |                  | 5     | 0        | 0         | 0.169  | 0.5    | 500    | 97%  | 50  | 150  | 0%   |   |
| Chloroform                     | A            | ug/L         | 118.39682  | 4.7358728      |                  | 5     | 0        | 0         | 0.0789 | 0.5    | 500    | 95%  | 50  | 150  | 0%   |   |
| Chloromethane                  | A            | ug/L         | 114.27651  | 4.5710604      |                  | 5     | 0        | 0         | 0.162  | 0.5    | 500    | 91%  | 50  | 150  | 0%   |   |
| cis-1,2-Dichloroethene         | A            | ug/L         | 122.15956  | 4.8863824      |                  | 5     | 0        | 0         | 0.108  | 0.5    | 500    | 98%  | 50  | 150  | 0%   |   |
| cis-1,3-Dichloropropene        | A            | ug/L         | 119.11853  | 4.7647412      |                  | 5     | 0        | 0         | 0.073  | 0.5    | 500    | 95%  | 50  | 150  | 0%   |   |
| Dibromomethane                 | A            | ug/L         | 120.85967  | 4.8343868      |                  | 5     | 0        | 0         | 0.147  | 0.5    | 500    | 97%  | 50  | 150  | 0%   |   |
| Dichlorodifluoromethane        | A            | ug/L         | 114.70512  | 4.5882048      |                  | 5     | 0        | 0         | 0.175  | 0.5    | 500    | 92%  | 50  | 150  | 0%   |   |
| Ethylbenzene                   | A            | ug/L         | 121.63922  | 4.8655688      |                  | 5     | 0        | 0         | 0.0836 | 0.5    | 500    | 97%  | 50  | 150  | 0%   |   |
| m+p-Xylenes                    | A            | ug/L         | 248.2876   | 9.931504       |                  | 10    | 0        | 0         | 0.15   | 0.5    | 1000   | 99%  | 50  | 150  | 0%   |   |
| Methyl ethyl ketone            | A            | ug/L         | 1168.59215 | 46.743686      |                  | 50    | 0        | 0         | 1.77   | 10     | 5000   | 93%  | 50  | 150  | 0%   |   |
| Methyl tert-butyl ether (MTBE) | A            | ug/L         | 119.22551  | 4.7690204      |                  | 5     | 0        | 0         | 0.101  | 0.5    | 500    | 95%  | 50  | 150  | 0%   |   |
| Methylene chloride             | A            | ug/L         | 114.81968  | 4.5927872      |                  | 5     | 0        | 0         | 0.338  | 0.5    | 500    | 92%  | 50  | 150  | 0%   |   |
| o-Xylene                       | A            | ug/L         | 123.16365  | 4.926546       |                  | 5     | 0        | 0         | 0.0604 | 0.5    | 500    | 99%  | 50  | 150  | 0%   |   |
| Styrene                        | A            | ug/L         | 126.27154  | 5.0508616      |                  | 5     | 0        | 0         | 0.067  | 0.5    | 500    | 101% | 50  | 150  | 0%   |   |
| Tetrachloroethene              | A            | ug/L         | 119.752    | 4.79008        |                  | 5     | 0        | 0         | 0.0671 | 0.5    | 500    | 96%  | 50  | 150  | 0%   |   |
| Toluene                        | A            | ug/L         | 123.86607  | 4.9546428      |                  | 5     | 0        | 0         | 0.0679 | 0.5    | 500    | 99%  | 50  | 150  | 0%   |   |
| trans-1,2-Dichloroethene       | A            | ug/L         | 120.86833  | 4.8347332      |                  | 5     | 0        | 0         | 0.125  | 0.5    | 500    | 97%  | 50  | 150  | 0%   |   |

| Seq No                    | Lab ID       | Test Code    | Sample Typ | File ID        | Analysis Date    | DF    | Batch ID | Prep Date | SPKref | RPDref | pmoist |      |     |      |      |   |
|---------------------------|--------------|--------------|------------|----------------|------------------|-------|----------|-----------|--------|--------|--------|------|-----|------|------|---|
| 14973528                  | CCV010722_CI | VOC-8260-W-Q | CCV        | DA5975C\VG010' | 1/7/2022 6:29:09 | 1     | R373037  |           | 0      | 0      |        |      |     |      |      |   |
| Analyte                   | T            | Units        | RAW        | Final          | Text             | Spike | SPKref   | RPDref    | MDL    | PQL    | UQL    | %REC | LOW | HIGH | %RPD | Q |
| trans-1,3-Dichloropropene | A            | ug/L         | 124.4317   | 4.977268       |                  | 5     | 0        | 0         | 0.0846 | 0.5    | 500    | 100% | 50  | 150  | 0%   |   |
| Trichloroethene           | A            | ug/L         | 122.28717  | 4.8914868      |                  | 5     | 0        | 0         | 0.0993 | 0.5    | 500    | 98%  | 50  | 150  | 0%   |   |
| Trichlorofluoromethane    | A            | ug/L         | 105.41691  | 4.2166764      |                  | 5     | 0        | 0         | 0.134  | 0.5    | 500    | 84%  | 50  | 150  | 0%   |   |
| Vinyl chloride            | A            | ug/L         | 117.75408  | 4.7101632      |                  | 5     | 0        | 0         | 0.153  | 0.5    | 500    | 94%  | 50  | 150  | 0%   |   |
| 1,4-Dichlorobenzene-d4    | I            | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 0   | 0    | 0%   |   |
| Chlorobenzene-d5          | I            | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 0   | 0    | 0%   |   |
| Fluorobenzene             | I            | ug/L         | 250        | 10             |                  | 0     | 0        | 0         | 0      | 0      | 500    | 0%   | 0   | 0    | 0%   |   |
| Xylenes, Total            | M            | ug/L         | 371.45125  | 14.85805       |                  | 15    | 0        | 0         | 0.0604 | 0.5    | 1500   | 99%  | 50  | 150  | 0%   |   |
| 1,2-Dichloroethane-d4     | S            | ug/L         | 273.91948  | 10.9567792     |                  | 10    | 0        | 0         | 0.229  | 0.5    | 500    | 110% | 50  | 150  | 0%   |   |
| Dibromofluoromethane      | S            | ug/L         | 267.46235  | 10.698494      |                  | 10    | 0        | 0         | 0.129  | 0.5    | 500    | 107% | 50  | 150  | 0%   |   |
| p-Bromofluorobenzene      | S            | ug/L         | 268.41426  | 10.7365704     |                  | 10    | 0        | 0         | 0.149  | 0.5    | 500    | 107% | 50  | 150  | 0%   |   |
| Toluene-d8                | S            | ug/L         | 272.36346  | 10.8945384     |                  | 10    | 0        | 0         | 0.23   | 0.5    | 500    | 109% | 50  | 150  | 0%   |   |

DATAFILE HEADERS FROM C:\MSDCHEM\1\DATA\VG010722

Data file Name : C:\MSDCHEM\1\DATA\VG010722\07JAN01.D  
Sample Name : PRIMER  
Operator : MSC  
Date injected : 7 Jan 2022 8:36 am  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 1

---

Data file Name : C:\MSDCHEM\1\DATA\VG010722\07JAN02.D  
Sample Name : BFB010722\_  
Operator : MSC  
Date injected : 7 Jan 2022 9:03 am  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 2

---

Data file Name : C:\MSDCHEM\1\DATA\VG010722\07JAN03.D  
Sample Name : CCV010722\_  
Operator : MSC  
Date injected : 7 Jan 2022 9:43 am  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 3

---

Data file Name : C:\MSDCHEM\1\DATA\VG010722\07JAN04.D  
Sample Name : LCS010722\_  
Operator : MSC  
Date injected : 7 Jan 2022 10:50 am  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 4

---

Data file Name : C:\MSDCHEM\1\DATA\VG010722\07JAN05.D

Sample Name : BLK  
Operator : MSC  
Date injected : 7 Jan 2022 11:17 am  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 5

---

Data file Name : C:\MSDCHEM\1\DATA\VG010722\07JAN06.D  
Sample Name : MBLK010722\_  
Operator : MSC  
Date injected : 7 Jan 2022 11:45 am  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 6

---

Data file Name : C:\MSDCHEM\1\DATA\VG010722\07JAN07.D  
Sample Name : B22010214-002A  
Operator : MSC  
Date injected : 7 Jan 2022 12:24 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 7

---

Data file Name : C:\MSDCHEM\1\DATA\VG010722\07JAN08.D  
Sample Name : B22010219-002A  
Operator : MSC  
Date injected : 7 Jan 2022 12:52 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 8

---

Data file Name : C:\MSDCHEM\1\DATA\VG010722\07JAN09.D  
Sample Name : B22010226-002A  
Operator : MSC  
Date injected : 7 Jan 2022 1:19 pm

Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 9

---

Data file Name : C:\MSDCHEM\1\DATA\VG010722\07JAN10.D  
Sample Name : B22010214-002A  
Operator : MSC  
Date injected : 7 Jan 2022 1:46 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 10

---

Data file Name : C:\MSDCHEM\1\DATA\VG010722\07JAN11.D  
Sample Name : B22010219-001F  
Operator : MSC  
Date injected : 7 Jan 2022 2:14 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 11

---

Data file Name : C:\MSDCHEM\1\DATA\VG010722\07JAN12.D  
Sample Name : B22010213-002C  
Operator : MSC  
Date injected : 7 Jan 2022 2:41 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 12

---

Data file Name : C:\MSDCHEM\1\DATA\VG010722\07JAN13.D  
Sample Name : BLK  
Operator : MSC  
Date injected : 7 Jan 2022 3:08 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616

Start Time : 0.840  
End Time : 16.498  
Vial Number : 13

---

Data file Name : C:\MSDCHEM\1\DATA\VG010722\07JAN14.D  
Sample Name : B22010214-001F  
Operator : MSC  
Date injected : 7 Jan 2022 3:35 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 14

---

Data file Name : C:\MSDCHEM\1\DATA\VG010722\07JAN15.D  
Sample Name : B22010262-001F  
Operator : MSC  
Date injected : 7 Jan 2022 4:03 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 15

---

Data file Name : C:\MSDCHEM\1\DATA\VG010722\07JAN16.D  
Sample Name : BLK  
Operator : MSC  
Date injected : 7 Jan 2022 4:40 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.839  
End Time : 16.498  
Vial Number : 16

---

Data file Name : C:\MSDCHEM\1\DATA\VG010722\07JAN17.D  
Sample Name : B22010219-001FMS  
Operator : MSC  
Date injected : 7 Jan 2022 5:07 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 17



-----  
Data file Name : C:\MSDCHEM\1\DATA\VG010722\07JAN18.D  
Sample Name : B22010219-001FMSD  
Operator : MSC  
Date injected : 7 Jan 2022 5:34 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 18  
-----



Data file Name : C:\MSDCHEM\1\DATA\VG010722\07JAN19.D  
Sample Name : BLK  
Operator : MSC  
Date injected : 7 Jan 2022 6:01 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 19  
-----

Data file Name : C:\MSDCHEM\1\DATA\VG010722\07JAN20.D  
Sample Name : CCV010722\_Closing  
Operator : MSC  
Date injected : 7 Jan 2022 6:29 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 20  
-----

Data file Name : C:\MSDCHEM\1\DATA\VG010722\07JAN21.D  
Sample Name : BLK  
Operator : MSC  
Date injected : 7 Jan 2022 6:56 pm  
Instrument : VOA5975C  
Method used : 5975CACQF  
No of spectra : 5616  
Start Time : 0.840  
End Time : 16.498  
Vial Number : 21  
-----

# Tune Evaluation Report

Data Path: D:\Org\Data\VOA5975C\VG010722\07JAN02.D  
 Acq on: 1/7/2022 9:03:26 AM  
 Operator: MSC  
 Sample: BFB010722\_  
 Inst Name: VOA5975C  
 ALS Vial: 2  
 Method: \\MASSHUNTER\Org\Data\Methods\BFBapex.m

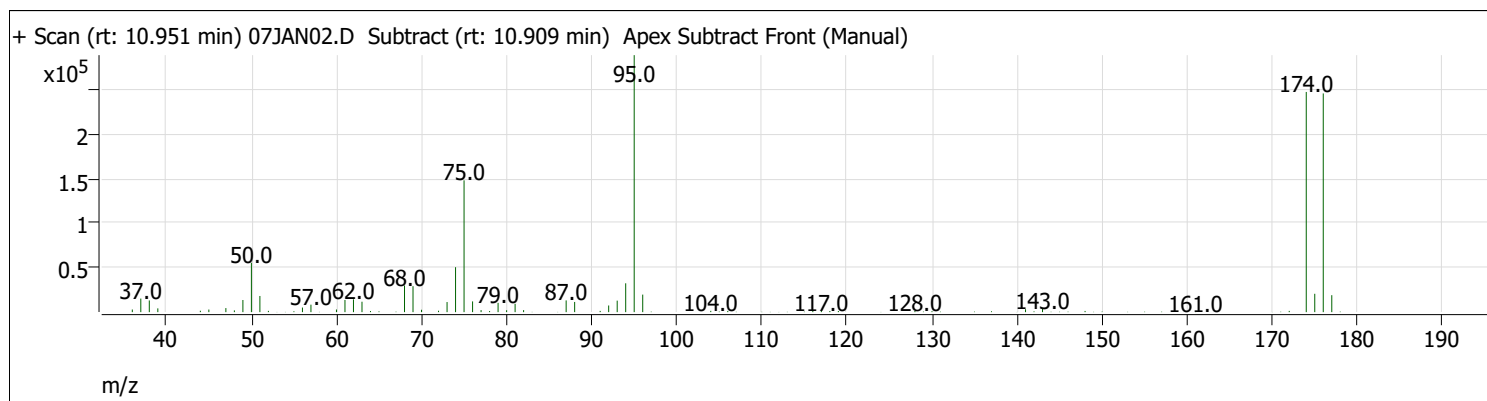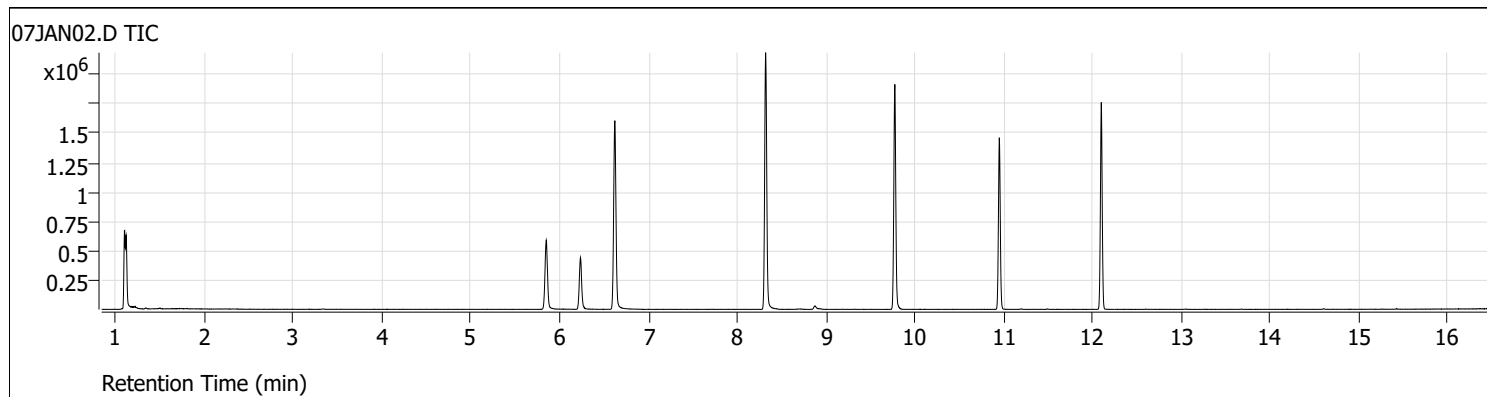

| Target Mass | Rel. To Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|-----------|
| 50          | 95           | 15           | 40           | 19.2      | 55384   | Pass      |
| 75          | 95           | 30           | 60           | 51.3      | 147840  | Pass      |
| 95          | 95           | 100          | 100          | 100.0     | 288256  | Pass      |
| 96          | 95           | 5            | 9            | 6.8       | 19656   | Pass      |
| 173         | 174          | 0            | 2            | 0.0       | 0       | Pass      |
| 174         | 95           | 50           | 100          | 85.7      | 246976  | Pass      |
| 175         | 174          | 5            | 9            | 8.3       | 20592   | Pass      |
| 176         | 174          | 95           | 101          | 99.3      | 245312  | Pass      |
| 177         | 176          | 5            | 9            | 7.7       | 19000   | Pass      |

# Continuing Calibration Report

**Batch Name** D:\Org\Data\VOA5975C\VG010722\QuantResults\VG010722\_8260B.batch.bin  
**Method File** \\MASSHUNTER\Org\Data\Methods\Quant\VOA5975C\VOA5975C\_010422\_CAL\VOA5975C\_8260B\_SHT\_DoD\_L4\_010422.m  
**Daily CC** D:\Org\Data\VOA5975C\VG01072207JAN03.D

| Level name | Injection Time      | Calibration Files                              |
|------------|---------------------|------------------------------------------------|
| 1          | 1/4/2022 3:33:04 PM | D:\Org\Data\VOA5975C\VG010422\04JAN10.D        |
| 2          | 1/4/2022 4:00:35 PM | D:\Org\Data\VOA5975C\VG010422\04JAN11.D        |
| 3          | 1/4/2022 4:28:05 PM | D:\Org\Data\VOA5975C\VG010422\04JAN12.D        |
| 4          | 1/4/2022 4:55:32 PM | D:\Org\Data\VOA5975C\VG010422\04JAN13.D        |
| 5          | 1/4/2022 5:50:25 PM | D:\Org\Data\VOA5975C\VG010422\04JAN15.D        |
| 6          | 1/4/2022 6:45:10 PM | D:\Org\Data\VOA5975C\VG010422\04JAN17.D        |
| 7          | 1/4/2022 7:39:45 PM | D:\Org\Data\VOA5975C\VG010422\04JAN19.D        |
| 8          | 1/4/2022 8:34:31 PM | D:\Org\Data\VOA5975C\VG010422\04JAN21.D        |
| CC         | 1/7/2022 9:43:06 AM | D:\Org\Data\VOA5975C\VG010722\07JAN03.D <===== |

| ISTD Compound:         | Avg Resp | Mid Resp | CC Resp | Area%  | A/M |
|------------------------|----------|----------|---------|--------|-----|
| Fluorobenzene          | 805964   | 778120   | 868396  | 111.60 | M   |
| Chlorobenzene-d5       | 305684   | 300356   | 338774  | 112.79 | M   |
| 1,4-Dichlorobenzene-d4 | 252451   | 248636   | 271840  | 109.33 | M   |

| Target Compound                | AvgRF/R2 | CC RF    | Exp. Conc | Calc. Conc | %Dev   | Area%  | Curve Fit |
|--------------------------------|----------|----------|-----------|------------|--------|--------|-----------|
| -----ISTD-----                 |          |          |           |            |        |        |           |
| Dichlorodifluoromethane        | 0.3276   | 0.3000   | 125.00    | 114.49     | 8.41   | 94.45  | Avg RF    |
| Chloromethane                  | 0.3976   | 0.3703   | 125.00    | 116.40     | 6.88   | 100.11 | Avg RF    |
| Vinyl chloride                 | 0.3578   | 0.3477   | 125.00    | 121.48     | 2.81   | 101.77 | Avg RF    |
| Bromomethane                   | 0.1600   | 0.1693   | 125.00    | 132.28     | -5.82  | 112.81 | Avg RF    |
| Chloroethane                   | 0.1771   | 0.1673   | 125.00    | 118.04     | 5.56   | 101.69 | Avg RF    |
| Trichlorofluoromethane         | 0.4441   | 0.3994   | 125.00    | 112.42     | 10.07  | 91.85  | Avg RF    |
| 1,1-Dichloroethene             | 0.2518   | 0.2447   | 125.00    | 121.47     | 2.82   | 106.85 | Avg RF    |
| Methylene chloride             | 0.3712   | 0.3545   | 125.00    | 119.36     | 4.51   | 113.78 | Avg RF    |
| trans-1,2-Dichloroethene       | 0.2569   | 0.2578   | 125.00    | 125.43     | -0.35  | 111.48 | Avg RF    |
| Methyl tert-butyl ether (MTBE) | 0.3321   | 0.3396   | 125.00    | 127.82     | -2.26  | 106.02 | Avg RF    |
| 1,1-Dichloroethane             | 0.4782   | 0.4891   | 125.00    | 127.83     | -2.27  | 114.13 | Avg RF    |
| 2,2-Dichloropropane            | 0.3583   | 0.3729   | 125.00    | 130.08     | -4.07  | 115.94 | Avg RF    |
| cis-1,2-Dichloroethene         | 0.2605   | 0.2682   | 125.00    | 128.71     | -2.97  | 116.38 | Avg RF    |
| Methyl ethyl ketone            | 0.0353   | 0.0355 # | 1250.00   | 1257.21    | -0.58  | 114.36 | Avg RF    |
| Bromochloromethane             | 0.1079   | 0.1110   | 125.00    | 128.60     | -2.88  | 114.86 | Avg RF    |
| Chloroform                     | 0.4759   | 0.4629   | 125.00    | 121.57     | 2.74   | 111.88 | Avg RF    |
| 1,1,1-Trichloroethane          | 0.4460   | 0.4463   | 125.00    | 125.09     | -0.07  | 111.25 | Avg RF    |
| Dibromofluoromethane           | 0.2355   | 0.2633   | 250.00    | 279.47     | -11.79 | 256.01 | Avg RF    |
| Carbon tetrachloride           | 0.4394   | 0.4228   | 125.00    | 120.28     | 3.78   | 106.17 | Avg RF    |
| 1,1-Dichloropropene            | 0.3792   | 0.3811   | 125.00    | 125.61     | -0.49  | 110.56 | Avg RF    |
| 1,2-Dichloroethane-d4          | 0.1017   | 0.1142   | 250.00    | 280.59     | -12.24 | 253.68 | Avg RF    |
| Benzene                        | 0.9954   | 1.0119   | 125.00    | 127.07     | -1.66  | 114.58 | Avg RF    |
| 1,2-Dichloroethane             | 0.2693   | 0.2665   | 125.00    | 123.72     | 1.03   | 110.36 | Avg RF    |
| -----ISTD-----                 |          |          |           |            |        |        |           |
| Trichloroethene                | 0.7540   | 0.7286   | 125.00    | 120.79     | 3.37   | 108.14 | Avg RF    |
| 1,2-Dichloropropane            | 0.6632   | 0.6756   | 125.00    | 127.33     | -1.87  | 115.37 | Avg RF    |
| Dibromomethane                 | 0.2803   | 0.2729   | 125.00    | 121.69     | 2.65   | 113.76 | Avg RF    |
| Bromodichloromethane           | 0.7735   | 0.7668   | 125.00    | 123.91     | 0.87   | 112.29 | Avg RF    |
| cis-1,3-Dichloropropene        | 0.8745   | 0.8551   | 125.00    | 122.22     | 2.22   | 111.92 | Avg RF    |
| Toluene-d8                     | 2.4091   | 2.5975   | 250.00    | 269.54     | -7.82  | 245.67 | Avg RF    |
| Toluene                        | 1.6274   | 1.6559   | 125.00    | 127.19     | -1.75  | 114.62 | Avg RF    |
| trans-1,3-Dichloropropene      | 0.6225   | 0.6351   | 125.00    | 127.53     | -2.02  | 116.03 | Avg RF    |
| 1,1,2-Trichloroethane          | 0.3242   | 0.3204   | 125.00    | 123.52     | 1.18   | 116.28 | Avg RF    |
| Tetrachloroethene              | 0.6639   | 0.6258   | 125.00    | 117.83     | 5.73   | 108.63 | Avg RF    |

# Continuing Calibration Report

| Target Compound           | AvgRF/R2       | CC RF  | Exp. Conc | Calc. Conc | %Dev   | Area%  | Curve Fit |
|---------------------------|----------------|--------|-----------|------------|--------|--------|-----------|
| 1,3-Dichloropropane       | 0.6378         | 0.6355 | 125.00    | 124.56     | 0.36   | 111.92 | Avg RF    |
| Chlorodibromomethane      | 0.5068         | 0.5066 | 125.00    | 124.97     | 0.03   | 114.40 | Avg RF    |
| 1,2-Dibromoethane         | 0.3545         | 0.3552 | 125.00    | 125.23     | -0.18  | 116.09 | Avg RF    |
| Chlorobenzene             | 1.7817         | 1.7567 | 125.00    | 123.25     | 1.40   | 112.88 | Avg RF    |
| 1,1,1,2-Tetrachloroethane | 0.6228         | 0.5884 | 125.00    | 118.09     | 5.53   | 109.64 | Avg RF    |
| Ethylbenzene              | 3.0900         | 3.0635 | 125.00    | 123.93     | 0.86   | 111.80 | Avg RF    |
| m+p-Xylenes               | 1.2008         | 1.2117 | 250.00    | 252.27     | -0.91  | 111.42 | Avg RF    |
| o-Xylene                  | 1.0690         | 1.0664 | 125.00    | 124.70     | 0.24   | 111.84 | Avg RF    |
| Styrene                   | 1.7211         | 1.7876 | 125.00    | 129.83     | -3.86  | 112.83 | Avg RF    |
| 1,4-Dichlorobenzene-d4    | -----ISTD----- |        |           |            |        |        |           |
| Bromoform                 | 0.3199         | 0.3294 | 125.00    | 128.72     | -2.98  | 114.33 | Avg RF    |
| p-Bromofluorobenzene      | 0.9159         | 1.0133 | 250.00    | 276.61     | -10.64 | 241.07 | Avg RF    |
| Bromobenzene              | 0.8091         | 0.8422 | 125.00    | 130.12     | -4.09  | 111.93 | Avg RF    |
| 1,1,2,2-Tetrachloroethane | 0.4657         | 0.4865 | 125.00    | 130.60     | -4.48  | 116.10 | Avg RF    |
| 1,2,3-Trichloropropane    | 0.1246         | 0.1295 | 125.00    | 129.90     | -3.92  | 53.15  | Avg RF    |
| 2-Chlorotoluene           | 0.8050         | 0.8325 | 125.00    | 129.26     | -3.41  | 110.47 | Avg RF    |
| 4-Chlorotoluene           | 2.6247         | 2.7862 | 125.00    | 132.69     | -6.15  | 112.66 | Avg RF    |
| 1,3-Dichlorobenzene       | 1.4756         | 1.4739 | 125.00    | 124.86     | 0.11   | 109.23 | Avg RF    |
| 1,4-Dichlorobenzene       | 1.5046         | 1.5178 | 125.00    | 126.10     | -0.88  | 109.13 | Avg RF    |
| 1,2-Dichlorobenzene       | 1.2470         | 1.2379 | 125.00    | 124.08     | 0.74   | 110.48 | Avg RF    |

A -- against Average; M -- against Mid Point; P -- against Previous CC in the Method;

# Continuing Calibration Report

**Batch Name** D:\Org\Data\VOA5975C\VG010722\QuantResults\VG010722\_8260B.batch.bin  
**Method File** \\MASSHUNTER\Org\Data\Methods\Quant\VOA5975C\VOA5975C\_010422\_CAL\VOA5975C\_8260B\_SHT\_DoD\_L4\_010422.m  
**Daily CC** D:\Org\Data\VOA5975C\VG01072207JAN20.D

| Level name | Injection Time      | Calibration Files                              |
|------------|---------------------|------------------------------------------------|
| 1          | 1/4/2022 3:33:04 PM | D:\Org\Data\VOA5975C\VG010422\04JAN10.D        |
| 2          | 1/4/2022 4:00:35 PM | D:\Org\Data\VOA5975C\VG010422\04JAN11.D        |
| 3          | 1/4/2022 4:28:05 PM | D:\Org\Data\VOA5975C\VG010422\04JAN12.D        |
| 4          | 1/4/2022 4:55:32 PM | D:\Org\Data\VOA5975C\VG010422\04JAN13.D        |
| 5          | 1/4/2022 5:50:25 PM | D:\Org\Data\VOA5975C\VG010422\04JAN15.D        |
| 6          | 1/4/2022 6:45:10 PM | D:\Org\Data\VOA5975C\VG010422\04JAN17.D        |
| 7          | 1/4/2022 7:39:45 PM | D:\Org\Data\VOA5975C\VG010422\04JAN19.D        |
| 8          | 1/4/2022 8:34:31 PM | D:\Org\Data\VOA5975C\VG010422\04JAN21.D        |
| CC         | 1/7/2022 6:29:09 PM | D:\Org\Data\VOA5975C\VG010722\07JAN20.D <===== |

| ISTD Compound:         | Avg Resp | Mid Resp | CC Resp | Area%  | A/M |
|------------------------|----------|----------|---------|--------|-----|
| Fluorobenzene          | 805964   | 778120   | 875212  | 112.48 | M   |
| Chlorobenzene-d5       | 305684   | 300356   | 332712  | 110.77 | M   |
| 1,4-Dichlorobenzene-d4 | 252451   | 248636   | 273694  | 110.08 | M   |

| Target Compound                | AvgRF/R2 | CC RF    | Exp. Conc | Calc. Conc | %Dev  | Area%  | Curve Fit |
|--------------------------------|----------|----------|-----------|------------|-------|--------|-----------|
| -----ISTD-----                 |          |          |           |            |       |        |           |
| Fluorobenzene                  |          |          |           |            |       |        |           |
| Dichlorodifluoromethane        | 0.3276   | 0.3006   | 125.00    | 114.71     | 8.24  | 95.38  | Avg RF    |
| Chloromethane                  | 0.3976   | 0.3635   | 125.00    | 114.28     | 8.58  | 99.05  | Avg RF    |
| Vinyl chloride                 | 0.3578   | 0.3371   | 125.00    | 117.75     | 5.80  | 99.42  | Avg RF    |
| Bromomethane                   | 0.1600   | 0.1591   | 125.00    | 124.27     | 0.58  | 106.81 | Avg RF    |
| Chloroethane                   | 0.1771   | 0.1720   | 125.00    | 121.35     | 2.92  | 105.36 | Avg RF    |
| Trichlorofluoromethane         | 0.4441   | 0.3745   | 125.00    | 105.42     | 15.67 | 86.81  | Avg RF    |
| 1,1-Dichloroethene             | 0.2518   | 0.2393   | 125.00    | 118.79     | 4.97  | 105.31 | Avg RF    |
| Methylene chloride             | 0.3712   | 0.3410   | 125.00    | 114.82     | 8.14  | 110.31 | Avg RF    |
| trans-1,2-Dichloroethene       | 0.2569   | 0.2484   | 125.00    | 120.87     | 3.31  | 108.27 | Avg RF    |
| Methyl tert-butyl ether (MTBE) | 0.3321   | 0.3167   | 125.00    | 119.23     | 4.62  | 99.67  | Avg RF    |
| 1,1-Dichloroethane             | 0.4782   | 0.4784   | 125.00    | 125.06     | -0.05 | 112.53 | Avg RF    |
| 2,2-Dichloropropane            | 0.3583   | 0.3490   | 125.00    | 121.75     | 2.60  | 109.36 | Avg RF    |
| cis-1,2-Dichloroethene         | 0.2605   | 0.2546   | 125.00    | 122.16     | 2.27  | 111.33 | Avg RF    |
| Methyl ethyl ketone            | 0.0353   | 0.0330 # | 1250.00   | 1168.59    | 6.51  | 107.13 | Avg RF    |
| Bromochloromethane             | 0.1079   | 0.0996 # | 125.00    | 115.33     | 7.74  | 103.81 | Avg RF    |
| Chloroform                     | 0.4759   | 0.4508   | 125.00    | 118.40     | 5.28  | 109.81 | Avg RF    |
| 1,1,1-Trichloroethane          | 0.4460   | 0.4243   | 125.00    | 118.91     | 4.87  | 106.58 | Avg RF    |
| Dibromofluoromethane           | 0.2355   | 0.2520   | 250.00    | 267.46     | -6.98 | 246.94 | Avg RF    |
| Carbon tetrachloride           | 0.4394   | 0.4135   | 125.00    | 117.62     | 5.91  | 104.64 | Avg RF    |
| 1,1-Dichloropropene            | 0.3792   | 0.3637   | 125.00    | 119.87     | 4.11  | 106.34 | Avg RF    |
| 1,2-Dichloroethane-d4          | 0.1017   | 0.1115   | 250.00    | 273.92     | -9.57 | 249.59 | Avg RF    |
| Benzene                        | 0.9954   | 0.9757   | 125.00    | 122.53     | 1.98  | 111.34 | Avg RF    |
| 1,2-Dichloroethane             | 0.2693   | 0.2479   | 125.00    | 115.10     | 7.92  | 103.48 | Avg RF    |
| -----ISTD-----                 |          |          |           |            |       |        |           |
| Chlorobenzene-d5               |          |          |           |            |       |        |           |
| Trichloroethene                | 0.7540   | 0.7376   | 125.00    | 122.29     | 2.17  | 107.52 | Avg RF    |
| 1,2-Dichloropropane            | 0.6632   | 0.6568   | 125.00    | 123.79     | 0.97  | 110.16 | Avg RF    |
| Dibromomethane                 | 0.2803   | 0.2710   | 125.00    | 120.86     | 3.31  | 110.96 | Avg RF    |
| Bromodichloromethane           | 0.7735   | 0.7318   | 125.00    | 118.26     | 5.39  | 105.25 | Avg RF    |
| cis-1,3-Dichloropropene        | 0.8745   | 0.8334   | 125.00    | 119.12     | 4.71  | 107.12 | Avg RF    |
| Toluene-d8                     | 2.4091   | 2.6246   | 250.00    | 272.36     | -8.95 | 243.80 | Avg RF    |
| Toluene                        | 1.6274   | 1.6126   | 125.00    | 123.87     | 0.91  | 109.63 | Avg RF    |
| trans-1,3-Dichloropropene      | 0.6225   | 0.6197   | 125.00    | 124.43     | 0.45  | 111.18 | Avg RF    |
| 1,1,2-Trichloroethane          | 0.3242   | 0.3035   | 125.00    | 116.98     | 6.41  | 108.16 | Avg RF    |
| Tetrachloroethene              | 0.6639   | 0.6360   | 125.00    | 119.75     | 4.20  | 108.42 | Avg RF    |


# Continuing Calibration Report

| Target Compound           | AvgRF/R2       | CC RF  | Exp. Conc | Calc. Conc | %Dev  | Area%  | Curve Fit |
|---------------------------|----------------|--------|-----------|------------|-------|--------|-----------|
| 1,3-Dichloropropane       | 0.6378         | 0.6202 | 125.00    | 121.55     | 2.76  | 107.26 | Avg RF    |
| Chlorodibromomethane      | 0.5068         | 0.4792 | 125.00    | 118.20     | 5.44  | 106.27 | Avg RF    |
| 1,2-Dibromoethane         | 0.3545         | 0.3404 | 125.00    | 120.01     | 3.99  | 109.26 | Avg RF    |
| Chlorobenzene             | 1.7817         | 1.7257 | 125.00    | 121.08     | 3.14  | 108.90 | Avg RF    |
| 1,1,1,2-Tetrachloroethane | 0.6228         | 0.5805 | 125.00    | 116.52     | 6.79  | 106.25 | Avg RF    |
| Ethylbenzene              | 3.0900         | 3.0069 | 125.00    | 121.64     | 2.69  | 107.77 | Avg RF    |
| m+p-Xylenes               | 1.2008         | 1.1926 | 250.00    | 248.29     | 0.68  | 107.70 | Avg RF    |
| o-Xylene                  | 1.0690         | 1.0533 | 125.00    | 123.16     | 1.47  | 108.49 | Avg RF    |
| Styrene                   | 1.7211         | 1.7386 | 125.00    | 126.27     | -1.02 | 107.77 | Avg RF    |
| 1,4-Dichlorobenzene-d4    | -----ISTD----- |        |           |            |       |        |           |
| Bromoform                 | 0.3199         | 0.3093 | 125.00    | 120.83     | 3.33  | 108.06 | Avg RF    |
| p-Bromofluorobenzene      | 0.9159         | 0.9833 | 250.00    | 268.41     | -7.37 | 235.53 | Avg RF    |
| Bromobenzene              | 0.8091         | 0.8074 | 125.00    | 124.74     | 0.21  | 108.04 | Avg RF    |
| 1,1,2,2-Tetrachloroethane | 0.4657         | 0.4519 | 125.00    | 121.30     | 2.96  | 108.57 | Avg RF    |
| 1,2,3-Trichloropropane    | 0.1246         | 0.1146 | 125.00    | 114.98     | 8.02  | 47.36  | Avg RF    |
| 2-Chlorotoluene           | 0.8050         | 0.7985 | 125.00    | 123.99     | 0.81  | 106.69 | Avg RF    |
| 4-Chlorotoluene           | 2.6247         | 2.6529 | 125.00    | 126.34     | -1.07 | 108.00 | Avg RF    |
| 1,3-Dichlorobenzene       | 1.4756         | 1.4331 | 125.00    | 121.40     | 2.88  | 106.93 | Avg RF    |
| 1,4-Dichlorobenzene       | 1.5046         | 1.4536 | 125.00    | 120.76     | 3.39  | 105.22 | Avg RF    |
| 1,2-Dichlorobenzene       | 1.2470         | 1.1845 | 125.00    | 118.73     | 5.01  | 106.44 | Avg RF    |

A -- against Average; M -- against Mid Point; P -- against Previous CC in the Method;

# Quantitation Results Report (QT Reviewed)

|                |                                     |                   |                       |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File      | 07JAN03.D                           | Operator          | MSC                   |
| Acq. Method    | 5975CACQF.M                         | Acq. Date-Time    | 1/7/2022 9:43:06 AM   |
| Sample Name    | CCV010722_                          | Instrument        | VOA5975C              |
| Vial           | 3                                   | Multiplier        | 1.00                  |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m  | Comment           |                       |
| Tune File      | BFB_Atune3.u                        | Tune Date         | 10/11/2021 4:02:00 PM |
| Batch Name     | VG010722_8260B.batch.bin            | Last Calib Update | 3/2/2022 10:41:44 AM  |
| Ref Library    | \\MASSHUNTER\Org\Library\NIST129K.I |                   |                       |



| Compound                           | RT                   | QIon  | Resp.  | Conc.              | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|--------------------|-------|----------|
| <b>Internal Standards</b>          |                      |       |        |                    |       |          |
| M Fluorobenzene                    | 6.620                | 96.0  | 868396 | 250.0000           | ng    | -0.003   |
| M Chlorobenzene-d5                 | 9.774                | 82.0  | 338774 | 250.0000           | ng    | 0.003    |
| M 1,4-Dichlorobenzene-d4           | 12.100               | 152.0 | 271840 | 250.0000           | ng    | 0.000    |
| <b>System Monitoring Compounds</b> |                      |       |        |                    |       |          |
| S Dibromofluoromethane             | 5.848                | 113.0 | 228638 | 279.4685           | ng    | 0.003    |
| Spiked Amount: 250.000             | Range: 80.0 - 119.0% |       |        | Recovery = 111.79% |       |          |
| S 1,2-Dichloroethane-d4            | 6.233                | 67.0  | 99152  | 280.5917           | ng    | 0.000    |
| Spiked Amount: 250.000             | Range: 81.0 - 118.0% |       |        | Recovery = 112.24% |       |          |
| S Toluene-d8                       | 8.319                | 98.0  | 879956 | 269.5449           | ng    | 0.000    |
| Spiked Amount: 250.000             | Range: 89.0 - 112.0% |       |        | Recovery = 107.82% |       |          |
| S p-Bromofluorobenzene             | 10.954               | 95.0  | 275469 | 276.6060           | ng    | 0.000    |
| Spiked Amount: 250.000             | Range: 85.0 - 114.0% |       |        | Recovery = 110.64% |       |          |
| <b>Target Compounds</b>            |                      |       |        |                    |       |          |
| T Dichlorodifluoromethane          | 1.241                | 85.0  | 130281 | 114.4850           | ng    | 100      |
| T Chloromethane                    | 1.408                | 50.0  | 160773 | 116.3992           | ng    | 100      |
| T Vinyl chloride                   | 1.498                | 62.0  | 150982 | 121.4824           | ng    | 97       |
| T Bromomethane                     | 1.802                | 96.0  | 73513  | 132.2812           | ng    | 97       |
| T Chloroethane                     | 1.897                | 64.0  | 72630  | 118.0450           | ng    | 99       |
| T Trichlorofluoromethane           | 2.147                | 101.0 | 173418 | 112.4176           | ng    | 100      |
| T 1,1-Dichloroethene               | 2.702                | 96.0  | 106254 | 121.4726           | ng    | 97       |
| T Methylene chloride               | 3.330                | 49.0  | 153910 | 119.3588           | ng    | 99       |
| T trans-1,2-Dichloroethene         | 3.720                | 96.0  | 111936 | 125.4320           | ng    | 98       |
| T Methyl tert-butyl ether (MTBE)   | 3.751                | 73.0  | 147444 | 127.8241           | ng    | 98       |
| T 1,1-Dichloroethane               | 4.378                | 63.0  | 212345 | 127.8331           | ng    | 98       |
| T 2,2-Dichloropropane              | 5.190                | 77.0  | 161912 | 130.0823           | ng    | 99       |
| T cis-1,2-Dichloroethene           | 5.209                | 96.0  | 116451 | 128.7076           | ng    | 97       |
| T Methyl ethyl ketone              | 5.282                | 43.0  | 154077 | 1257.2149          | ng    | 98       |
| T Bromochloromethane               | 5.522                | 128.0 | 48203  | 128.6024           | ng    | 99       |
| T Chloroform                       | 5.653                | 83.0  | 200976 | 121.5715           | ng    | 99       |













# Quantitation Results Report (QT Reviewed)

| Compound                    | RT     | QIon  | Resp.  | Conc.    | Units | Dev(Min) |
|-----------------------------|--------|-------|--------|----------|-------|----------|
| T 1,1,1-Trichloroethane     | 5.834  | 97.0  | 193800 | 125.0917 | ng    | 98       |
| T Carbon tetrachloride      | 6.026  | 117.0 | 183596 | 120.2774 | ng    | 99       |
| T 1,1-Dichloropropene       | 6.038  | 75.0  | 165459 | 125.6069 | ng    | 99       |
| T Benzene                   | 6.280  | 78.0  | 439363 | 127.0728 | ng    | 100      |
| T 1,2-Dichloroethane        | 6.319  | 62.0  | 115719 | 123.7158 | ng    | 97       |
| T Trichloroethene           | 7.025  | 95.0  | 123412 | 120.7910 | ng    | 97       |
| T 1,2-Dichloropropane       | 7.270  | 63.0  | 114436 | 127.3316 | ng    | 98       |
| T Dibromomethane            | 7.401  | 93.0  | 46218  | 121.6934 | ng    | 97       |
| T Bromodichloromethane      | 7.585  | 83.0  | 129880 | 123.9145 | ng    | 98       |
| T cis-1,3-Dichloropropene   | 8.057  | 75.0  | 144840 | 122.2214 | ng    | 98       |
| T Toluene                   | 8.386  | 92.0  | 280492 | 127.1937 | ng    | 98       |
| T trans-1,3-Dichloropropene | 8.637  | 75.0  | 107578 | 127.5302 | ng    | 98       |
| T 1,1,2-Trichloroethane     | 8.818  | 83.0  | 54273  | 123.5213 | ng    | 95       |
| T Tetrachloroethene         | 8.938  | 163.8 | 106010 | 117.8337 | ng    | 99       |
| T 1,3-Dichloropropane       | 8.980  | 76.0  | 107647 | 124.5555 | ng    | 99       |
| T Chlorodibromomethane      | 9.200  | 129.0 | 85816  | 124.9678 | ng    | 96       |
| T 1,2-Dibromoethane         | 9.306  | 107.0 | 60164  | 125.2299 | ng    | 99       |
| T Chlorobenzene             | 9.802  | 112.0 | 297566 | 123.2509 | ng    | 99       |
| T 1,1,1,2-Tetrachloroethane | 9.892  | 131.0 | 99659  | 118.0854 | ng    | 100      |
| T Ethylbenzene              | 9.919  | 91.0  | 518912 | 123.9274 | ng    | 100      |
| T m+p-Xylenes               | 10.037 | 106.0 | 410489 | 252.2653 | ng    | 100      |
| T o-Xylene                  | 10.433 | 106.0 | 180632 | 124.6951 | ng    | 99       |
| T Styrene                   | 10.446 | 104.0 | 302796 | 129.8291 | ng    | 99       |
| T Bromoform                 | 10.628 | 172.5 | 44778  | 128.7230 | ng    | 99       |
| T Bromobenzene              | 11.093 | 156.0 | 114469 | 130.1161 | ng    | 98       |
| T 1,1,2,2-Tetrachloroethane | 11.110 | 83.0  | 66129  | 130.5981 | ng    | 96       |
| T 1,2,3-Trichloropropane    | 11.149 | 110.0 | 17600  | 129.9023 | ng    | 100      |
| T 2-Chlorotoluene           | 11.289 | 126.0 | 113150 | 129.2634 | ng    | 99       |
| T 4-Chlorotoluene           | 11.400 | 91.0  | 378702 | 132.6910 | ng    | 99       |
| T 1,3-Dichlorobenzene       | 12.033 | 146.0 | 200331 | 124.8574 | ng    | 99       |
| T 1,4-Dichlorobenzene       | 12.125 | 146.0 | 206297 | 126.0981 | ng    | 99       |
| T 1,2-Dichlorobenzene       | 12.493 | 146.0 | 168250 | 124.0802 | ng    | 99       |

(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (\*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak




# Quantitation Results Report (QT Reviewed)

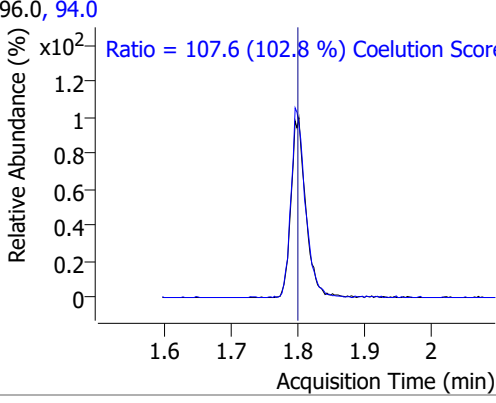
| Compound                                                                           | Conc.                                                                                | RT   | Dev(Min)                                                                              | Resp.  | QIon | QRatio                                       | Lower | Upper |
|------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------|------|---------------------------------------------------------------------------------------|--------|------|----------------------------------------------|-------|-------|
| Dichlorodifluoromethane                                                            | 114.4850                                                                             | 1.24 | 0.00                                                                                  | 130281 | 87.0 | 32.1                                         | 2.3   | 62.3  |
| + EIC (85.0) Scan 07JAN03.D                                                        |                                                                                      |      | 85.0, 87.0                                                                            |        |      | + Scan (1.219-1.339 min, 44 scans) 07JAN03.D |       |       |
|    |    |      |    |        |      |                                              |       |       |
| Chloromethane                                                                      | 116.3992                                                                             | 1.41 | 0.00                                                                                  | 160773 | 52.0 | 32.4                                         | 2.1   | 62.1  |
| + EIC (50.0) Scan 07JAN03.D                                                        |                                                                                      |      | 50.0, 52.0                                                                            |        |      | + Scan (1.375-1.484 min, 40 scans) 07JAN03.D |       |       |
|   |   |      |   |        |      |                                              |       |       |
| Vinyl chloride                                                                     | 121.4824                                                                             | 1.50 | 0.00                                                                                  | 150982 | 64.0 | 31.5                                         | 0.0   | 59.9  |
| + EIC (62.0) Scan 07JAN03.D                                                        |                                                                                      |      | 62.0, 64.0                                                                            |        |      | + Scan (1.470-1.595 min, 46 scans) 07JAN03.D |       |       |
|  |  |      |  |        |      |                                              |       |       |
| Bromomethane                                                                       | 132.2812                                                                             | 1.80 | 0.00                                                                                  | 73513  | 94.0 | 107.6                                        | 74.6  | 134.6 |
| + EIC (96.0) Scan 07JAN03.D                                                        |                                                                                      |      | 96.0, 94.0                                                                            |        |      | + Scan (1.763-1.888 min, 46 scans) 07JAN03.D |       |       |
|  |  |      |  |        |      |                                              |       |       |

# Quantitation Results Report (QT Reviewed)


| Compound     | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|----------|------|----------|-------|------|--------|-------|-------|
| Chloroethane | 118.0450 | 1.90 | 0.00     | 72630 | 66.0 | 30.7   | 0.1   | 60.1  |




| Compound               | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|------------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Trichlorofluoromethane | 112.4176 | 2.15 | 0.01     | 173418 | 103.0 | 64.3   | 34.2  | 94.2  |



| Compound           | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1-Dichloroethene | 121.4726 | 2.70 | 0.01     | 106254 | 61.0 | 185.3  | 150.3 | 210.3 |
|                    |          |      |          |        | 63.0 | 57.2   | 26.7  | 86.7  |




| Compound           | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| Methylene chloride | 119.3588 | 3.33 | -0.01    | 153910 | 84.0 | 67.3   | 36.9  | 96.9  |
|                    |          |      |          |        | 86.0 | 43.4   | 14.3  | 74.3  |




# Quantitation Results Report (QT Reviewed)


| Compound                 | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------------|----------|------|----------|--------|------|--------|-------|-------|
| trans-1,2-Dichloroethene | 125.4320 | 3.72 | 0.00     | 111936 | 61.0 | 156.2  | 123.9 | 183.9 |
|                          |          |      |          |        | 98.0 | 63.5   | 35.7  | 95.7  |

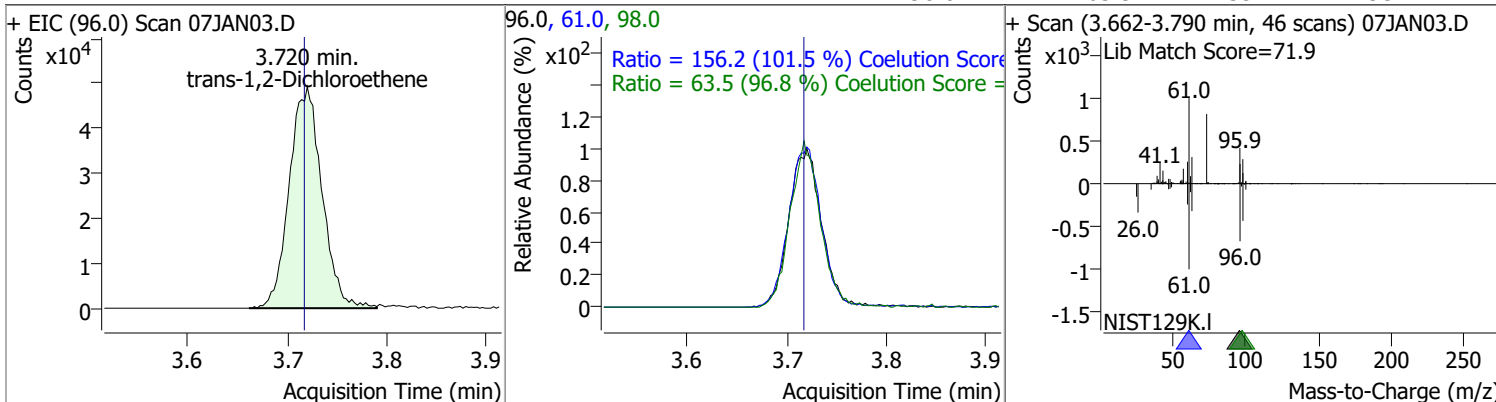

| Compound                       | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------------------|----------|------|----------|--------|------|--------|-------|-------|
| Methyl tert-butyl ether (MTBE) | 127.8241 | 3.75 | 0.00     | 147444 | 57.0 | 25.5   | 0.0   | 54.6  |




| Compound           | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1-Dichloroethane | 127.8331 | 4.38 | 0.00     | 212345 | 65.0 | 31.2   | 2.1   | 62.1  |
|                    |          |      |          |        | 83.0 | 12.9   | 0.0   | 43.7  |




# Quantitation Results Report (QT Reviewed)


| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 2,2-Dichloropropane | 130.0823 | 5.19 | -0.01    | 161912 | 41.0 | 67.1   | 36.5  | 96.5  |
|                     |          |      |          |        | 97.0 | 23.4   | 0.0   | 53.2  |

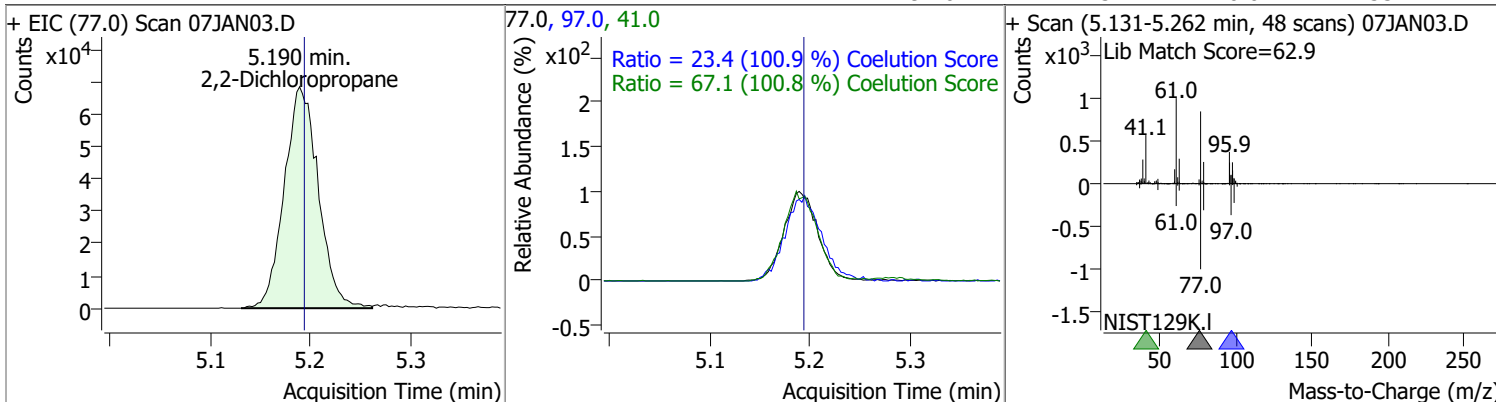


| Compound               | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,2-Dichloroethene | 128.7076 | 5.21 | -0.01    | 116451 | 61.0 | 163.2  | 137.2 | 197.2 |
|                        |          |      |          |        | 98.0 | 65.6   | 37.3  | 97.3  |

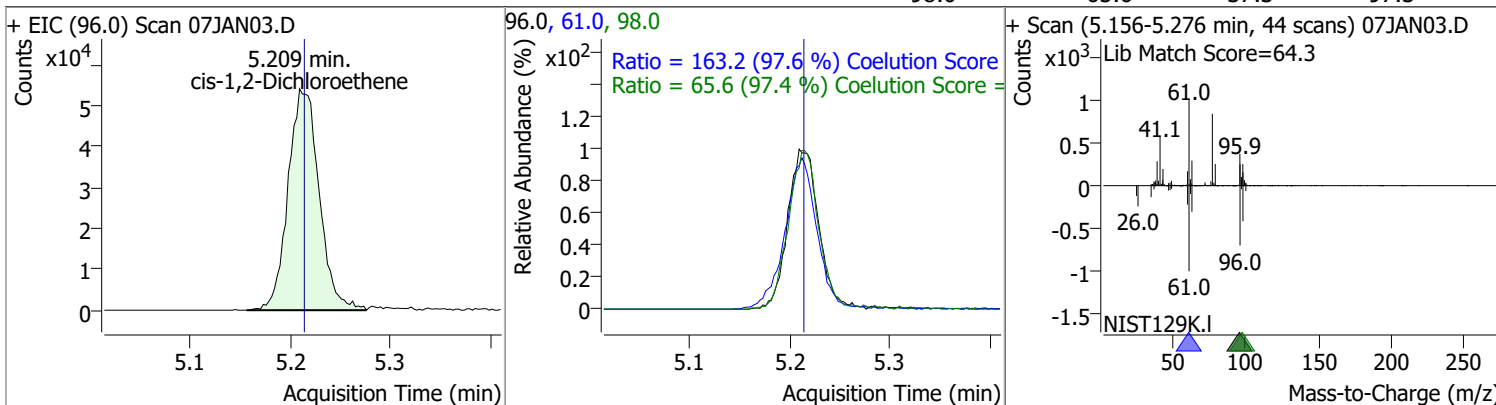





| Compound            | Conc.     | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|-----------|------|----------|--------|------|--------|-------|-------|
| Methyl ethyl ketone | 1257.2149 | 5.28 | 0.00     | 154077 | 72.0 | 20.2   | 0.0   | 51.3  |

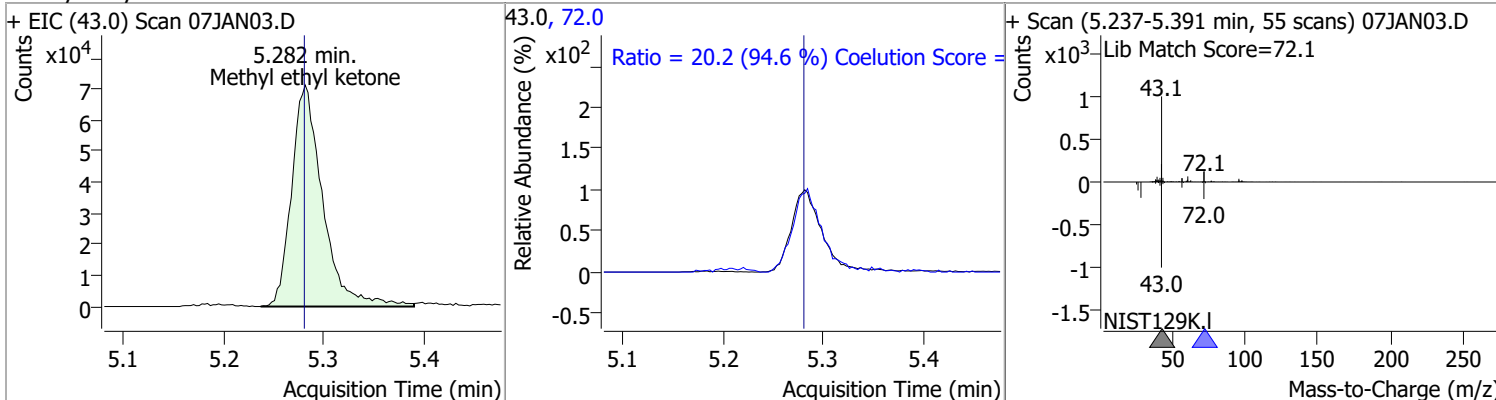

| Compound           | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|-------|------|--------|-------|-------|
| Bromochloromethane | 128.6024 | 5.52 | 0.00     | 48203 | 49.0 | 181.6  | 152.9 | 212.9 |

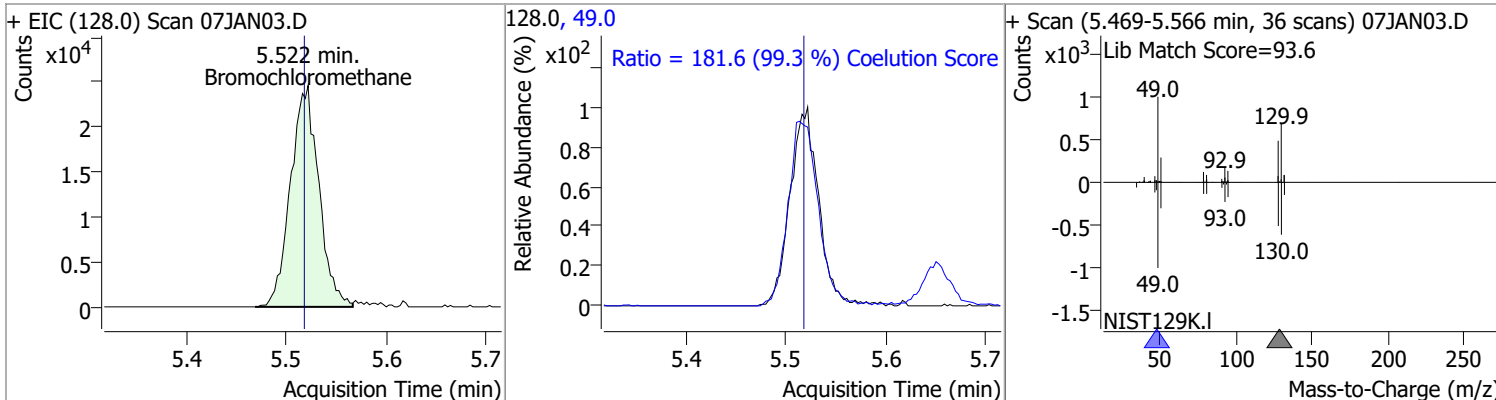


# Quantitation Results Report (QT Reviewed)




# Quantitation Results Report (QT Reviewed)


| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|-------|--------|-------|-------|
| 1,1-Dichloropropene | 125.6069 | 6.04 | 0.00     | 165459 | 110.0 | 35.3   | 5.9   | 65.9  |
|                     |          |      |          |        | 77.0  | 30.3   | 0.1   | 60.1  |

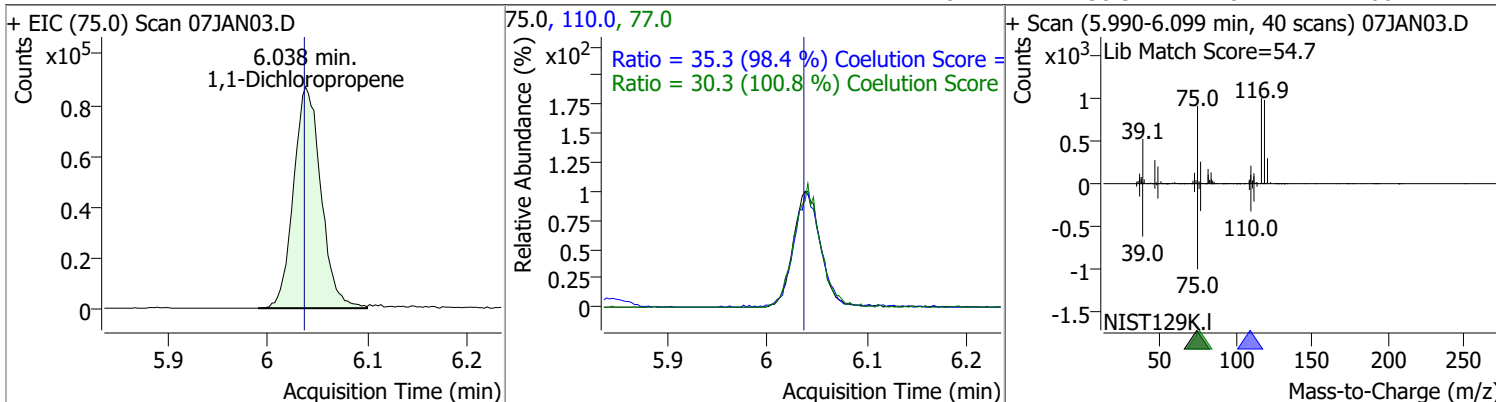


| Compound              | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 280.5917 | 6.23 | 0.00     | 99152 | 65.0 | 200.3  | 166.5 | 226.5 |

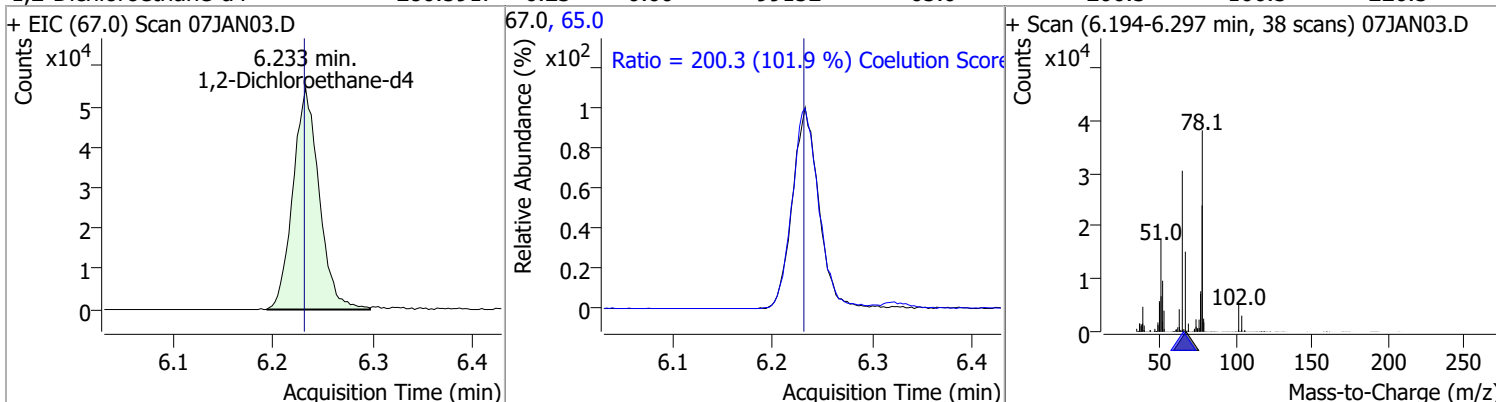

| Compound | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|----------|----------|------|----------|--------|------|--------|-------|-------|
| Benzene  | 127.0728 | 6.28 | 0.00     | 439363 | 77.0 | 23.3   | 0.0   | 53.5  |

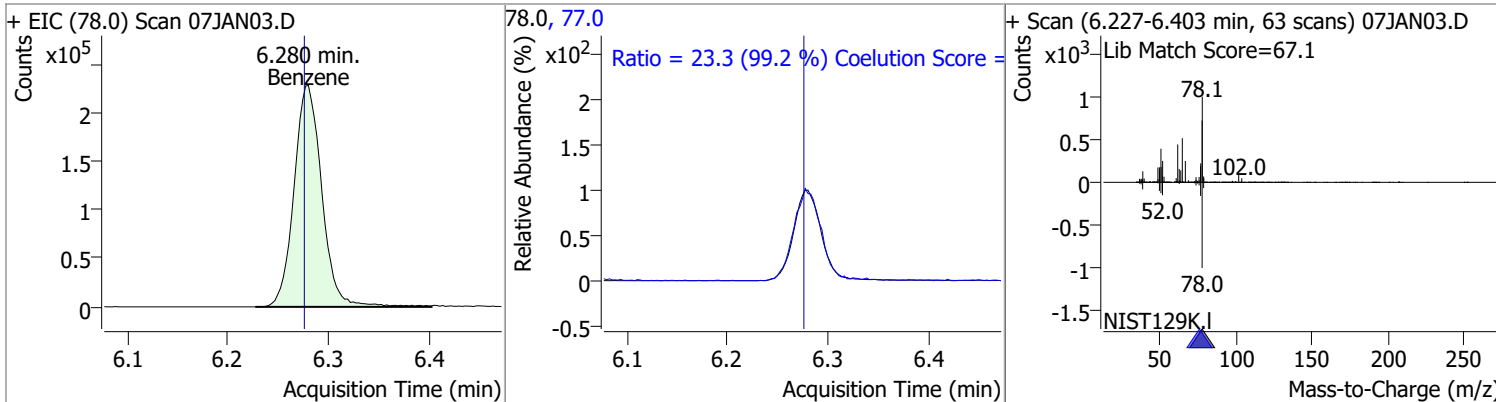


| Compound           | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloroethane | 123.7158 | 6.32 | 0.00     | 115719 | 64.0 | 32.1   | 0.0   | 59.9  |
|                    |          |      |          |        | 98.0 | 8.1    | 0.0   | 37.6  |




# Quantitation Results Report (QT Reviewed)


| Compound        | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|-----------------|----------|------|----------|--------|-------|--------|-------|-------|
| Trichloroethene | 120.7910 | 7.02 | -0.01    | 123412 | 130.0 | 105.0  | 71.5  | 131.5 |
|                 |          |      |          |        | 97.0  | 66.1   | 34.1  | 94.1  |

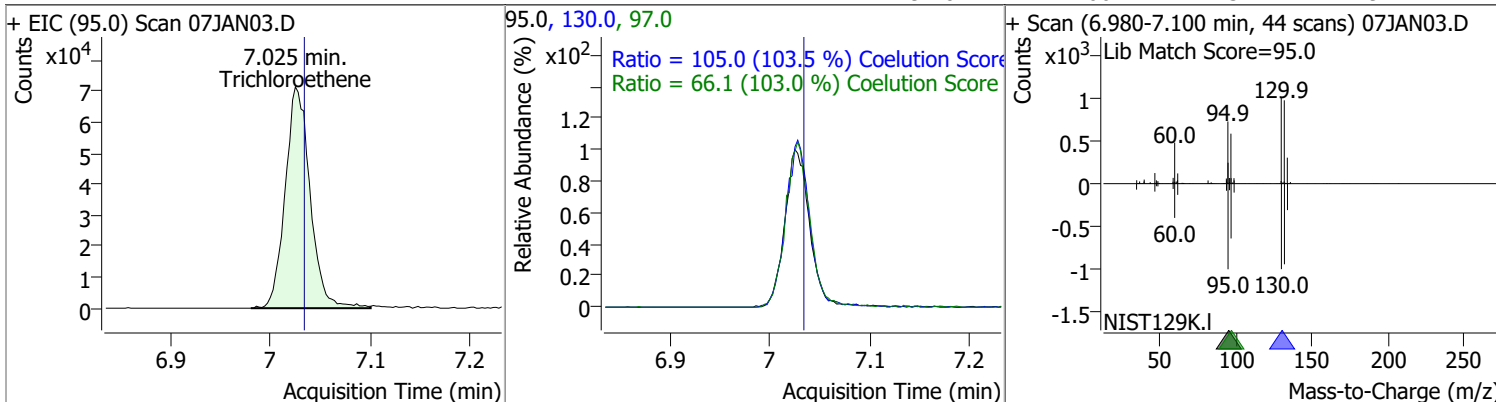

| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloropropane | 127.3316 | 7.27 | 0.00     | 114436 | 76.0 | 36.7   | 8.2   | 68.2  |



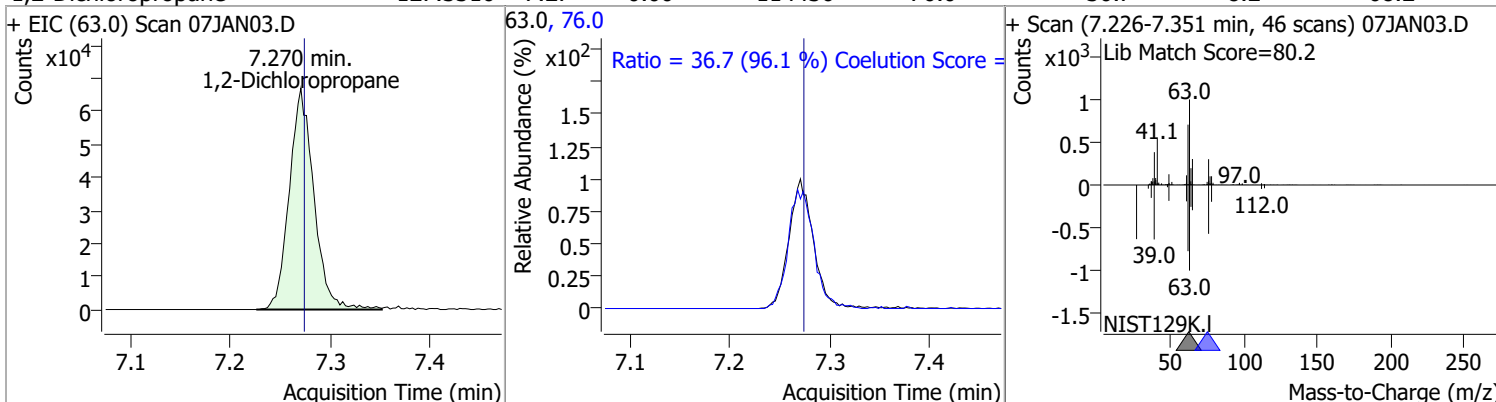


| Compound       | Conc.    | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|----------------|----------|------|----------|-------|-------|--------|-------|-------|
| Dibromomethane | 121.6934 | 7.40 | 0.00     | 46218 | 173.5 | 110.2  | 83.7  | 143.7 |
|                |          |      |          |       | 95.0  | 84.0   | 52.2  | 112.2 |



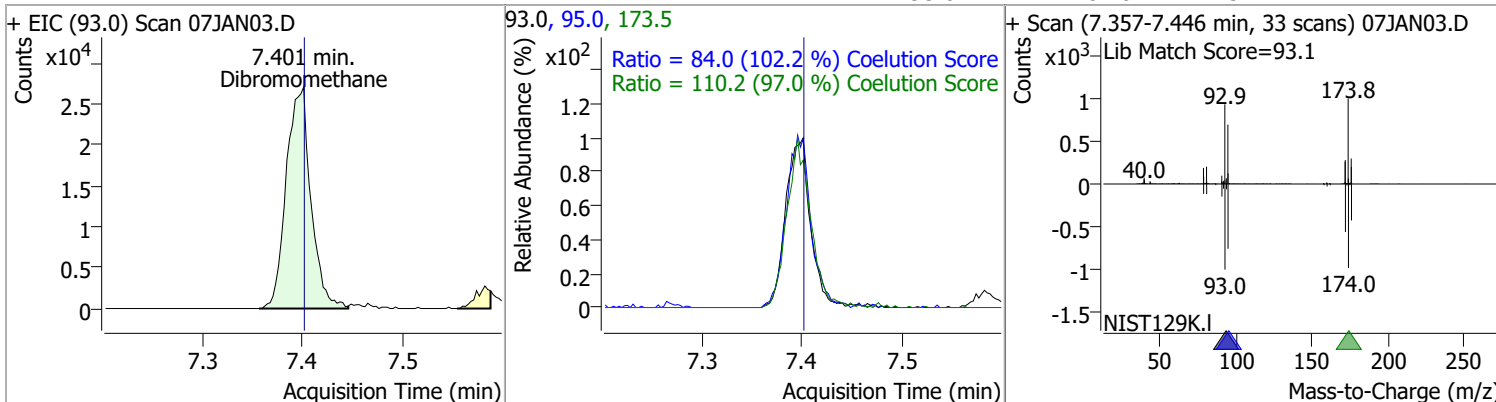


# Quantitation Results Report (QT Reviewed)




| Compound             | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Bromodichloromethane | 123.9145 | 7.59 | 0.00     | 129880 | 85.0  | 63.1   | 34.5  | 94.5  |
|                      |          |      |          |        | 127.0 | 8.6    | 0.0   | 39.6  |



| Compound                | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|-------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,3-Dichloropropene | 122.2214 | 8.06 | 0.00     | 144840 | 39.0 | 54.3   | 23.3  | 83.3  |
|                         |          |      |          |        | 77.0 | 32.5   | 1.0   | 61.0  |




| Compound   | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 269.5449 | 8.32 | 0.00     | 879956 | 100.0 | 64.1   | 34.4  | 94.4  |
|            |          |      |          |        | 99.0  | 9.6    | 0.0   | 39.6  |






# Quantitation Results Report (QT Reviewed)


| Compound | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|----------|----------|------|----------|--------|------|--------|-------|-------|
| Toluene  | 127.1937 | 8.39 | 0.00     | 280492 | 91.0 | 172.7  | 145.8 | 205.8 |

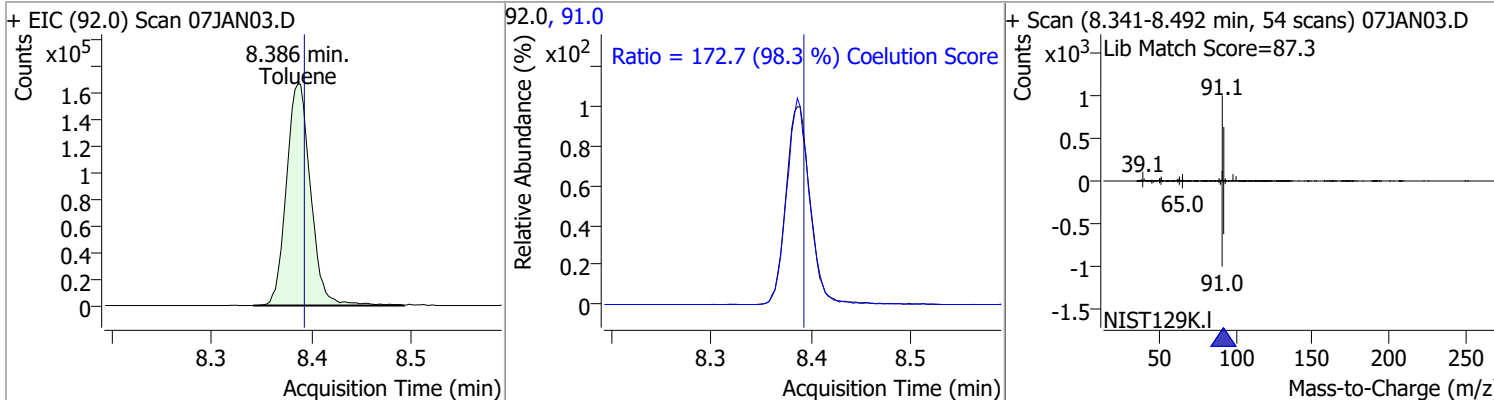

| Compound                  | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------------|----------|------|----------|--------|------|--------|-------|-------|
| trans-1,3-Dichloropropene | 127.5302 | 8.64 | 0.00     | 107578 | 39.0 | 53.1   | 23.4  | 83.4  |
|                           |          |      |          |        | 77.0 | 35.1   | 2.4   | 62.4  |

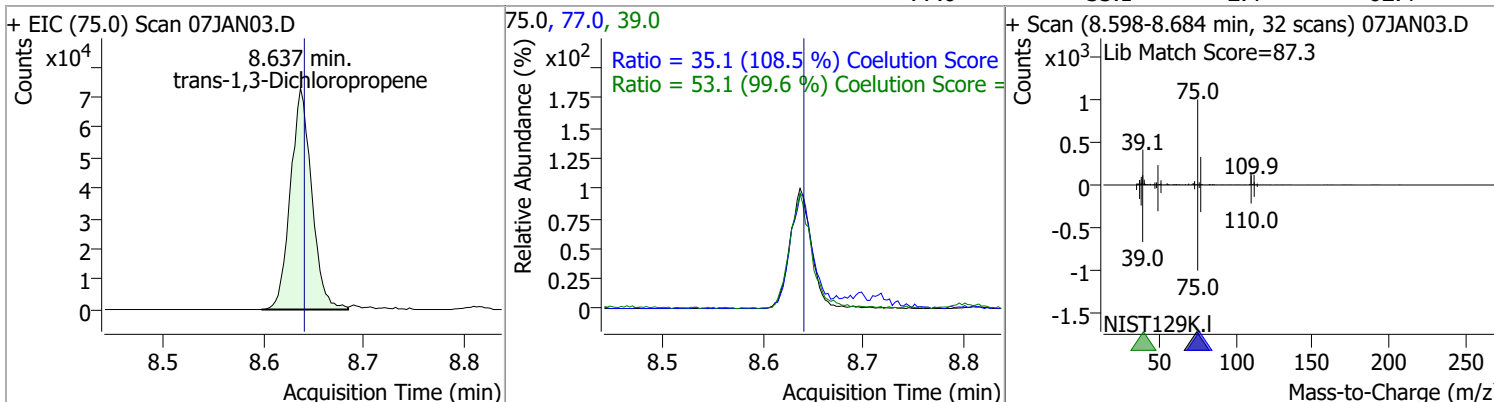


| Compound              | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,1,2-Trichloroethane | 123.5213 | 8.82 | 0.00     | 54273 | 97.0 | 111.4  | 84.6  | 144.6 |
|                       |          |      |          |       | 85.0 | 61.3   | 37.6  | 97.6  |

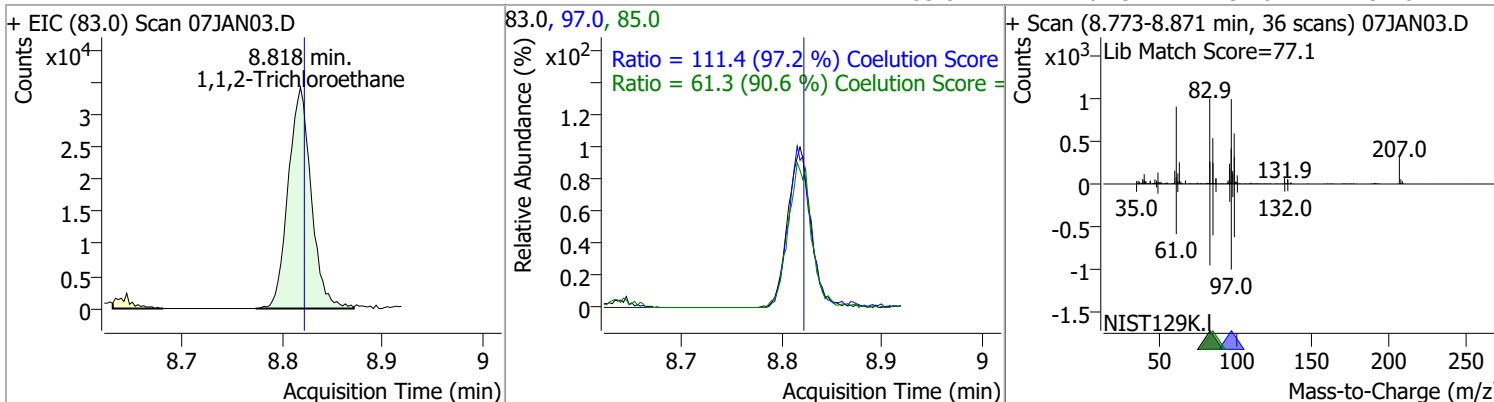


# Quantitation Results Report (QT Reviewed)


| Compound          | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|-------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Tetrachloroethene | 117.8337 | 8.94 | 0.00     | 106010 | 165.8 | 127.2  | 98.6  | 158.6 |
|                   |          |      |          |        | 129.0 | 89.7   | 61.5  | 121.5 |




| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,3-Dichloropropane | 124.5555 | 8.98 | 0.00     | 107647 | 78.0 | 32.4   | 2.9   | 62.9  |







| Compound             | Conc.    | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|----------------------|----------|------|----------|-------|-------|--------|-------|-------|
| Chlorodibromomethane | 124.9678 | 9.20 | -0.01    | 85816 | 127.0 | 74.9   | 48.0  | 108.0 |



| Compound          | Conc.    | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|-------------------|----------|------|----------|-------|-------|--------|-------|-------|
| 1,2-Dibromoethane | 125.2299 | 9.31 | 0.00     | 60164 | 109.0 | 95.8   | 64.5  | 124.5 |




# Quantitation Results Report (QT Reviewed)

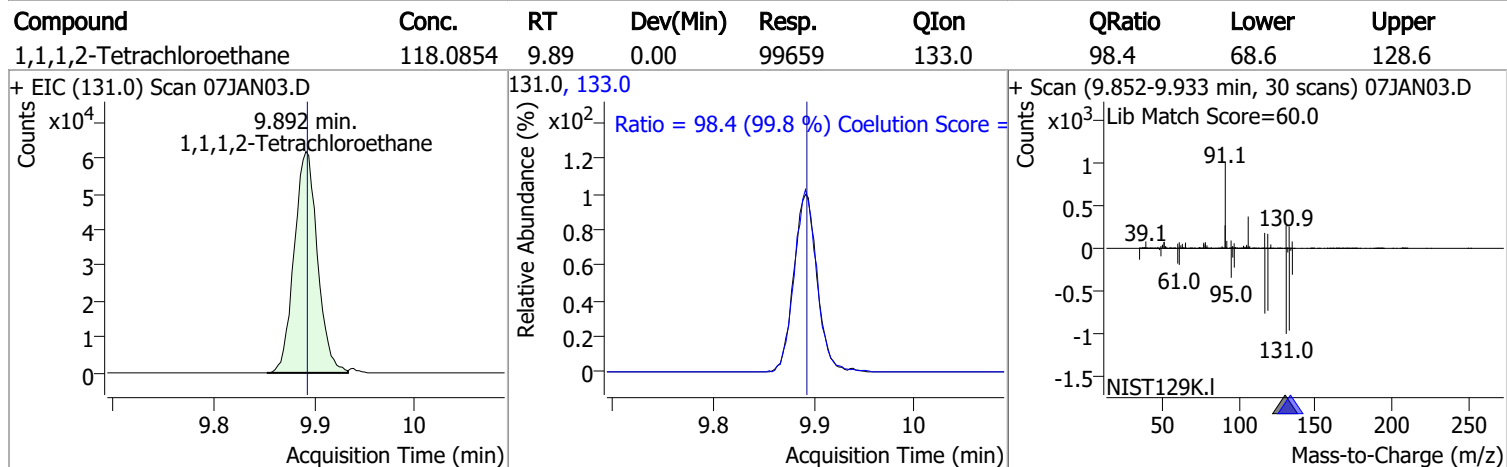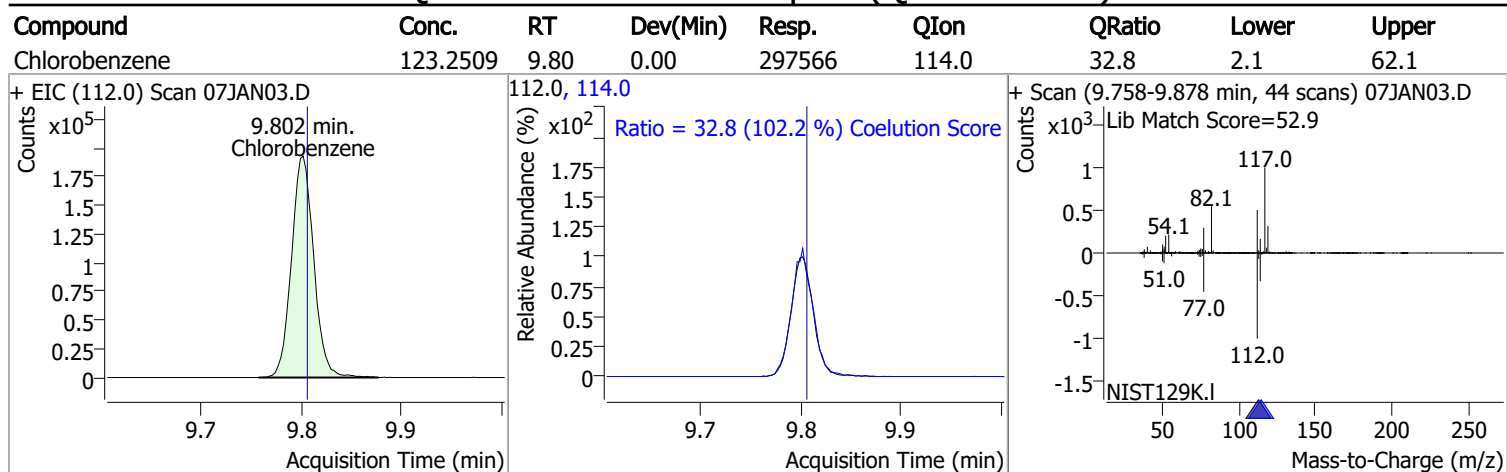


# Quantitation Results Report (QT Reviewed)


| Compound | Conc.    | RT    | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|----------|----------|-------|----------|--------|------|--------|-------|-------|
| o-Xylene | 124.6951 | 10.43 | 0.00     | 180632 | 91.0 | 214.8  | 183.1 | 243.1 |




| Compound | Conc.    | RT    | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|----------|----------|-------|----------|--------|------|--------|-------|-------|
| Styrene  | 129.8291 | 10.45 | 0.00     | 302796 | 78.0 | 50.0   | 19.6  | 79.6  |



| Compound  | Conc.    | RT    | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|-----------|----------|-------|----------|-------|-------|--------|-------|-------|
| Bromoform | 128.7230 | 10.63 | 0.00     | 44778 | 170.5 | 53.0   | 22.1  | 82.1  |
|           |          |       |          |       | 174.5 | 50.3   | 20.1  | 80.1  |




| Compound             | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 276.6060 | 10.95 | 0.00     | 275469 | 174.0 | 91.3   | 61.7  | 121.7 |
|                      |          |       |          |        | 176.0 | 89.0   | 60.6  | 120.6 |




# Quantitation Results Report (QT Reviewed)


| Compound     | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|--------------|----------|-------|----------|--------|-------|--------|-------|-------|
| Bromobenzene | 130.1161 | 11.09 | 0.00     | 114469 | 77.0  | 143.8  | 115.7 | 175.7 |
|              |          |       |          |        | 158.0 | 94.8   | 66.5  | 126.5 |




| Compound                  | Conc.    | RT    | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|----------|-------|----------|-------|------|--------|-------|-------|
| 1,1,2,2-Tetrachloroethane | 130.5981 | 11.11 | -0.01    | 66129 | 85.0 | 62.7   | 36.2  | 96.2  |



| Compound               | Conc.    | RT    | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|------------------------|----------|-------|----------|-------|-------|--------|-------|-------|
| 1,2,3-Trichloropropane | 129.9023 | 11.15 | 0.00     | 17600 | 112.0 | 63.4   | 33.5  | 93.5  |




| Compound        | Conc.    | RT    | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|-----------------|----------|-------|----------|--------|------|--------|-------|-------|
| 2-Chlorotoluene | 129.2634 | 11.29 | 0.00     | 113150 | 91.0 | 284.8  | 252.3 | 312.3 |




# Quantitation Results Report (QT Reviewed)


| Compound        | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|-----------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 4-Chlorotoluene | 132.6910 | 11.40 | 0.00     | 378702 | 126.0 | 31.1   | 1.7   | 61.7  |

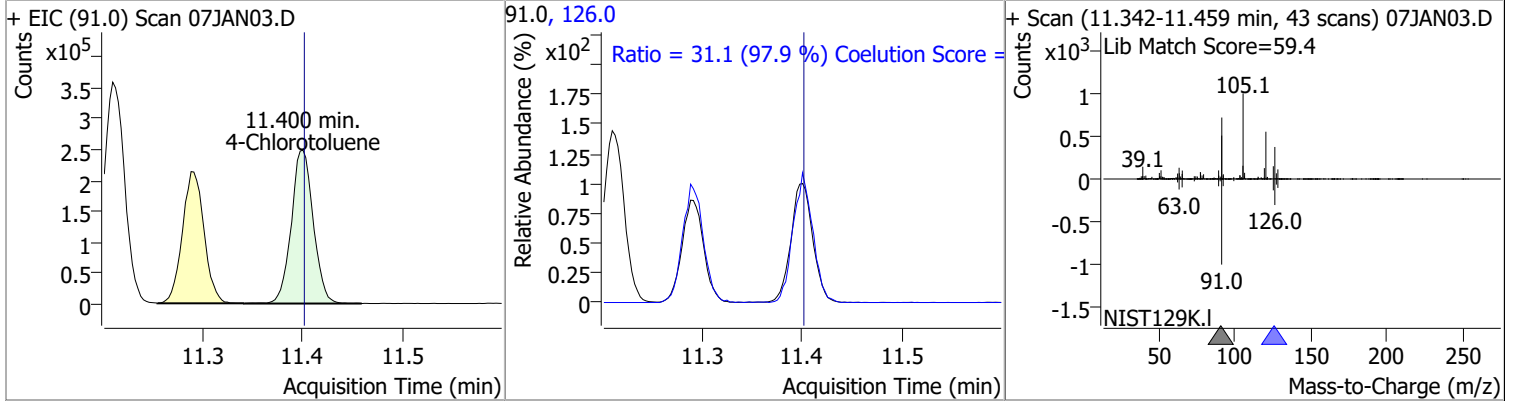

| Compound            | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,3-Dichlorobenzene | 124.8574 | 12.03 | 0.00     | 200331 | 148.0 | 64.2   | 33.6  | 93.6  |
|                     |          |       |          |        | 111.0 | 38.7   | 9.8   | 69.8  |






| Compound            | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,4-Dichlorobenzene | 126.0981 | 12.13 | 0.00     | 206297 | 148.0 | 64.4   | 33.1  | 93.1  |
|                     |          |       |          |        | 111.0 | 39.5   | 9.1   | 69.1  |




# Quantitation Results Report (QT Reviewed)

| Compound            | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,2-Dichlorobenzene | 124.0802 | 12.49 | 0.00     | 168250 | 148.0 | 64.5   | 33.9  | 93.9  |
|                     |          |       |          |        | 111.0 | 40.8   | 11.0  | 71.0  |

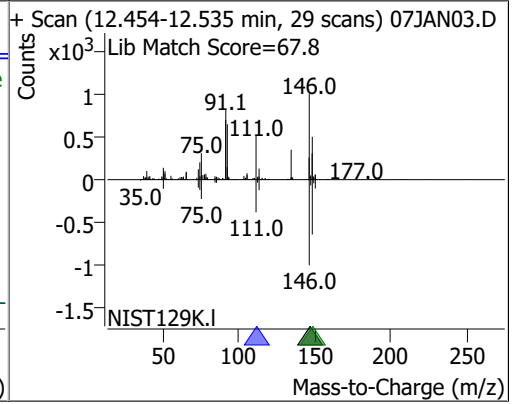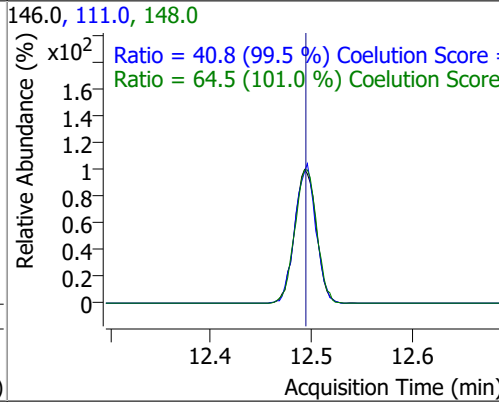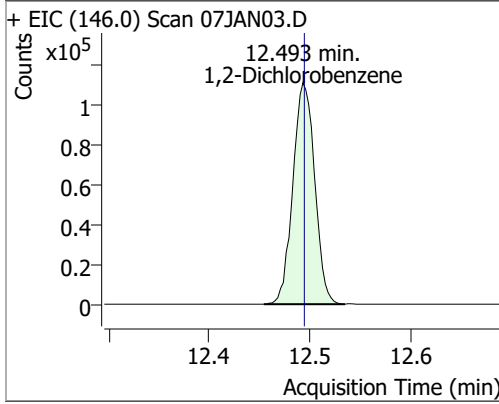

# Quantitation Results Report (QT Reviewed)

|                |                                     |                   |                       |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File      | 07JAN04.D                           | Operator          | MSC                   |
| Acq. Method    | 5975CACQF.M                         | Acq. Date-Time    | 1/7/2022 10:50:30 AM  |
| Sample Name    | LCS010722_                          | Instrument        | VOA5975C              |
| Vial           | 4                                   | Multiplier        | 1.00                  |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m  | Comment           |                       |
| Tune File      | BFB_Atune3.u                        | Tune Date         | 10/11/2021 4:02:00 PM |
| Batch Name     | VG010722_8260B.batch.bin            | Last Calib Update | 3/2/2022 10:41:44 AM  |
| Ref Library    | \\MASSHUNTER\Org\Library\NIST129K.I |                   |                       |

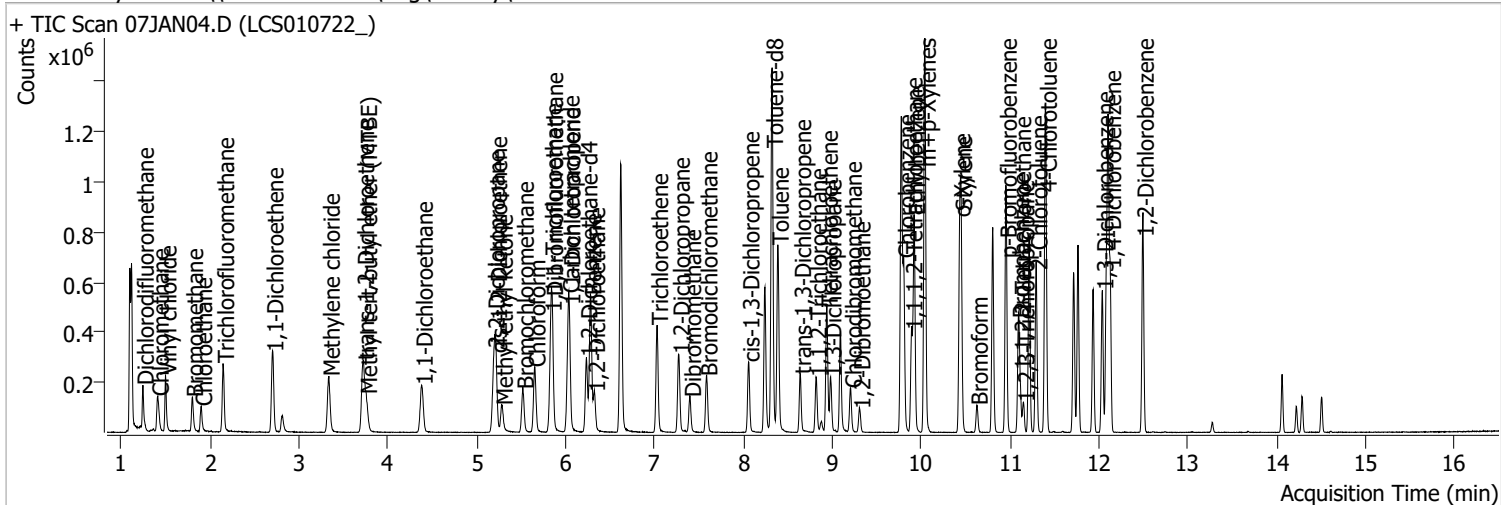

| Compound                           | RT                   | QIon  | Resp.  | Conc.              | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|--------------------|-------|----------|
| <b>Internal Standards</b>          |                      |       |        |                    |       |          |
| M Fluorobenzene                    | 6.620                | 96.0  | 907718 | 250.0000           | ng    | -0.003   |
| M Chlorobenzene-d5                 | 9.774                | 82.0  | 346586 | 250.0000           | ng    | 0.003    |
| M 1,4-Dichlorobenzene-d4           | 12.103               | 152.0 | 280949 | 250.0000           | ng    | 0.003    |
| <b>System Monitoring Compounds</b> |                      |       |        |                    |       |          |
| S Dibromofluoromethane             | 5.848                | 113.0 | 231280 | 270.4515           | ng    | 0.003    |
| Spiked Amount: 250.000             | Range: 80.0 - 119.0% |       |        | Recovery = 108.18% |       |          |
| S 1,2-Dichloroethane-d4            | 6.233                | 67.0  | 104500 | 282.9153           | ng    | 0.000    |
| Spiked Amount: 250.000             | Range: 81.0 - 118.0% |       |        | Recovery = 113.17% |       |          |
| S Toluene-d8                       | 8.321                | 98.0  | 905281 | 271.0520           | ng    | 0.003    |
| Spiked Amount: 250.000             | Range: 89.0 - 112.0% |       |        | Recovery = 108.42% |       |          |
| S p-Bromofluorobenzene             | 10.951               | 95.0  | 279940 | 271.9817           | ng    | -0.003   |
| Spiked Amount: 250.000             | Range: 85.0 - 114.0% |       |        | Recovery = 108.79% |       |          |
| <b>Target Compounds</b>            |                      |       |        |                    |       |          |
| T Dichlorodifluoromethane          | 1.244                | 85.0  | 123278 | 103.6382           | ng    | 99       |
| T Chloromethane                    | 1.411                | 50.0  | 156934 | 108.6978           | ng    | 99       |
| T Vinyl chloride                   | 1.498                | 62.0  | 154899 | 119.2350           | ng    | 97       |
| T Bromomethane                     | 1.799                | 96.0  | 70232  | 120.9026           | ng    | 99       |
| T Chloroethane                     | 1.899                | 64.0  | 70493  | 109.6085           | ng    | 97       |
| T Trichlorofluoromethane           | 2.145                | 101.0 | 181809 | 112.7515           | ng    | 99       |
| T 1,1-Dichloroethene               | 2.700                | 96.0  | 122201 | 133.6517           | ng    | 96       |
| T Methylene chloride               | 3.335                | 49.0  | 159195 | 118.1093           | ng    | 99       |
| T trans-1,2-Dichloroethene         | 3.720                | 96.0  | 121109 | 129.8320           | ng    | 97       |
| T Methyl tert-butyl ether (MTBE)   | 3.756                | 73.0  | 160126 | 132.8050           | ng    | 99       |
| T 1,1-Dichloroethane               | 4.381                | 63.0  | 227596 | 131.0789           | ng    | 100      |
| T 2,2-Dichloropropane              | 5.193                | 77.0  | 167542 | 128.7744           | ng    | 100      |
| T cis-1,2-Dichloroethene           | 5.218                | 96.0  | 122647 | 129.6836           | ng    | 98       |
| T Methyl ethyl ketone              | 5.282                | 43.0  | 145822 | 1138.3128          | ng    | 98       |
| T Bromochloromethane               | 5.519                | 128.0 | 47092  | 120.1958           | ng    | 93       |
| T Chloroform                       | 5.650                | 83.0  | 206280 | 119.3745           | ng    | 100      |











# Quantitation Results Report (QT Reviewed)

| Compound                    | RT     | QIon  | Resp.  | Conc.    | Units | Dev(Min) |
|-----------------------------|--------|-------|--------|----------|-------|----------|
| T 1,1,1-Trichloroethane     | 5.831  | 97.0  | 197819 | 122.1545 | ng    | 99       |
| T Carbon tetrachloride      | 6.032  | 117.0 | 187698 | 117.6380 | ng    | 99       |
| T 1,1-Dichloropropene       | 6.040  | 75.0  | 162591 | 118.0827 | ng    | 99       |
| T Benzene                   | 6.280  | 78.0  | 461197 | 127.6093 | ng    | 100      |
| T 1,2-Dichloroethane        | 6.319  | 62.0  | 119261 | 121.9792 | ng    | 100      |
| T Trichloroethene           | 7.028  | 95.0  | 131597 | 125.8989 | ng    | 99       |
| T 1,2-Dichloropropane       | 7.270  | 63.0  | 114080 | 124.0744 | ng    | 99       |
| T Dibromomethane            | 7.398  | 93.0  | 48238  | 124.1493 | ng    | 97       |
| T Bromodichloromethane      | 7.582  | 83.0  | 136799 | 127.5739 | ng    | 99       |
| T cis-1,3-Dichloropropene   | 8.057  | 75.0  | 142161 | 117.2568 | ng    | 99       |
| T Toluene                   | 8.386  | 92.0  | 291378 | 129.1519 | ng    | 99       |
| T trans-1,3-Dichloropropene | 8.637  | 75.0  | 113275 | 131.2571 | ng    | 95       |
| T 1,1,2-Trichloroethane     | 8.815  | 83.0  | 56261  | 125.1597 | ng    | 99       |
| T Tetrachloroethene         | 8.935  | 163.8 | 109421 | 118.8837 | ng    | 100      |
| T 1,3-Dichloropropane       | 8.980  | 76.0  | 107326 | 121.3850 | ng    | 99       |
| T Chlorodibromomethane      | 9.205  | 129.0 | 86224  | 122.7318 | ng    | 99       |
| T 1,2-Dibromoethane         | 9.306  | 107.0 | 60530  | 123.1519 | ng    | 100      |
| T Chlorobenzene             | 9.802  | 112.0 | 310348 | 125.6477 | ng    | 99       |
| T 1,1,1,2-Tetrachloroethane | 9.889  | 131.0 | 108057 | 125.1503 | ng    | 94       |
| T Ethylbenzene              | 9.919  | 91.0  | 539522 | 125.9452 | ng    | 99       |
| T m+p-Xylenes               | 10.039 | 106.0 | 417695 | 250.9079 | ng    | 99       |
| T o-Xylene                  | 10.430 | 106.0 | 192510 | 129.8994 | ng    | 100      |
| T Styrene                   | 10.449 | 104.0 | 316187 | 132.5150 | ng    | 100      |
| T Bromoform                 | 10.625 | 172.5 | 47153  | 131.1556 | ng    | 99       |
| T Bromobenzene              | 11.091 | 156.0 | 119622 | 131.5649 | ng    | 100      |
| T 1,1,2,2-Tetrachloroethane | 11.110 | 83.0  | 64431  | 123.1192 | ng    | 98       |
| T 1,2,3-Trichloropropane    | 11.149 | 110.0 | 17528  | 125.1764 | ng    | 99       |
| T 2-Chlorotoluene           | 11.294 | 126.0 | 117650 | 130.0465 | ng    | 97       |
| T 4-Chlorotoluene           | 11.400 | 91.0  | 398147 | 134.9812 | ng    | 100      |
| T 1,3-Dichlorobenzene       | 12.036 | 146.0 | 218804 | 131.9494 | ng    | 99       |
| T 1,4-Dichlorobenzene       | 12.125 | 146.0 | 217500 | 128.6355 | ng    | 99       |
| T 1,2-Dichlorobenzene       | 12.493 | 146.0 | 175961 | 125.5596 | ng    | 99       |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (\*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

# Quantitation Results Report (QT Reviewed)

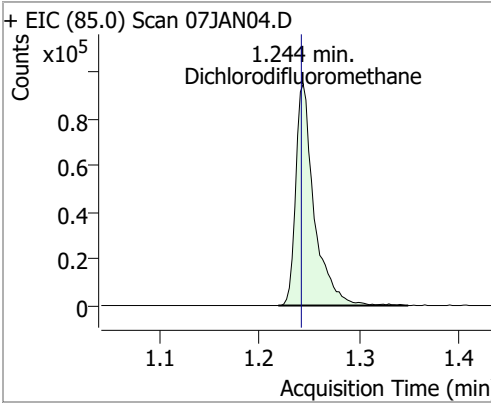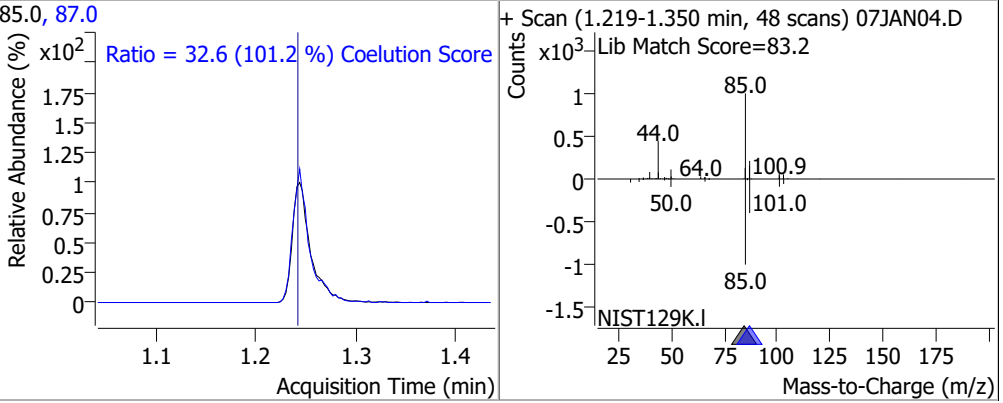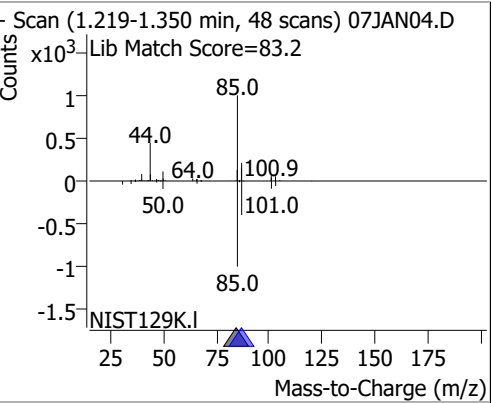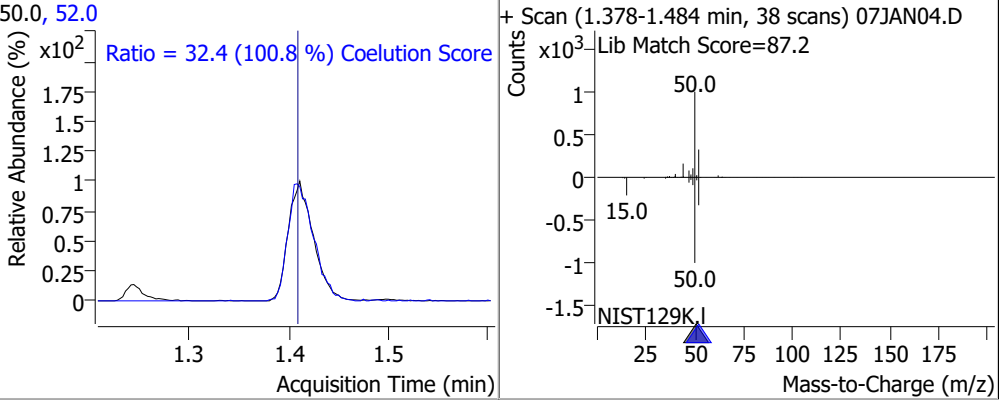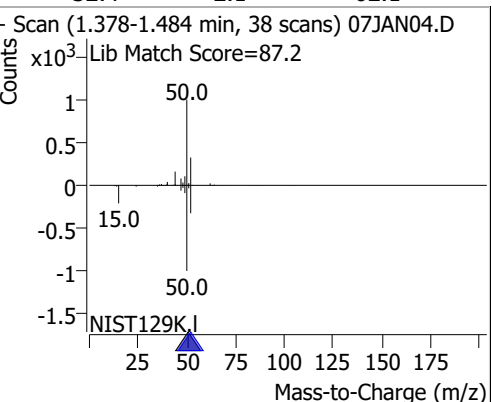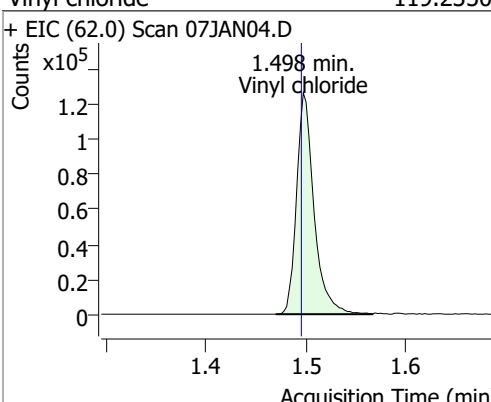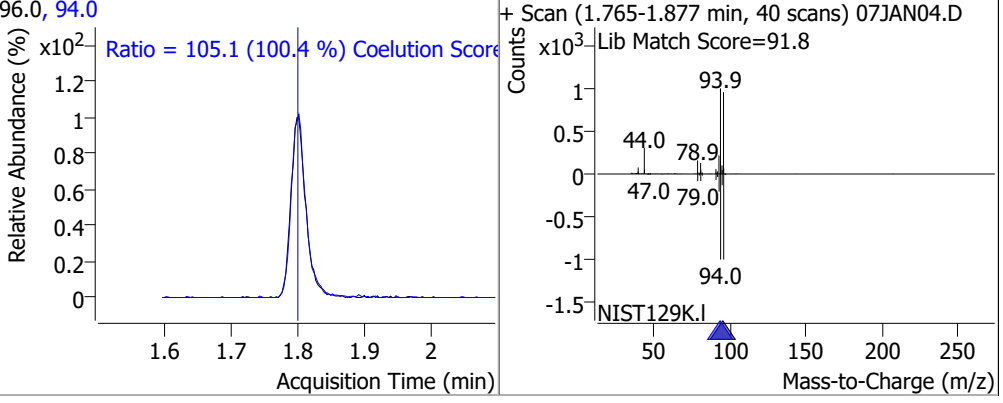
| Compound                                                                           | Conc.                                   | RT   | Dev(Min)                                                                             | Resp.  | QIon | QRatio                                       | Lower | Upper |
|------------------------------------------------------------------------------------|-----------------------------------------|------|--------------------------------------------------------------------------------------|--------|------|----------------------------------------------|-------|-------|
| Dichlorodifluoromethane                                                            | 103.6382                                | 1.24 | 0.00                                                                                 | 123278 | 87.0 | 32.6                                         | 2.3   | 62.3  |
| + EIC (85.0) Scan 07JAN04.D                                                        |                                         |      | 85.0, 87.0                                                                           |        |      | + Scan (1.219-1.350 min, 48 scans) 07JAN04.D |       |       |
|    | Ratio = 32.6 (101.2 %) Coelution Score  |      |    |        |      |                                              |       |       |
| Chloromethane                                                                      | 108.6978                                | 1.41 | 0.00                                                                                 | 156934 | 52.0 | 32.4                                         | 2.1   | 62.1  |
| + EIC (50.0) Scan 07JAN04.D                                                        |                                         |      | 50.0, 52.0                                                                           |        |      | + Scan (1.378-1.484 min, 38 scans) 07JAN04.D |       |       |
|   | Ratio = 32.4 (100.8 %) Coelution Score  |      |   |        |      |                                              |       |       |
| Vinyl chloride                                                                     | 119.2350                                | 1.50 | 0.00                                                                                 | 154899 | 64.0 | 31.4                                         | 0.0   | 59.9  |
| + EIC (62.0) Scan 07JAN04.D                                                        |                                         |      | 62.0, 64.0                                                                           |        |      | + Scan (1.470-1.567 min, 36 scans) 07JAN04.D |       |       |
|  | Ratio = 31.4 (105.0 %) Coelution Score  |      |  |        |      |                                              |       |       |
| Bromomethane                                                                       | 120.9026                                | 1.80 | 0.00                                                                                 | 70232  | 94.0 | 105.1                                        | 74.6  | 134.6 |
| + EIC (96.0) Scan 07JAN04.D                                                        |                                         |      | 96.0, 94.0                                                                           |        |      | + Scan (1.765-1.877 min, 40 scans) 07JAN04.D |       |       |
|  | Ratio = 105.1 (100.4 %) Coelution Score |      |  |        |      |                                              |       |       |

# Quantitation Results Report (QT Reviewed)


| Compound     | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|----------|------|----------|-------|------|--------|-------|-------|
| Chloroethane | 109.6085 | 1.90 | 0.01     | 70493 | 66.0 | 31.9   | 0.1   | 60.1  |




| Compound               | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|------------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Trichlorofluoromethane | 112.7515 | 2.14 | 0.00     | 181809 | 103.0 | 65.1   | 34.2  | 94.2  |



| Compound           | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1-Dichloroethene | 133.6517 | 2.70 | 0.00     | 122201 | 61.0 | 173.9  | 150.3 | 210.3 |
|                    |          |      |          |        | 63.0 | 54.1   | 26.7  | 86.7  |




| Compound           | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| Methylene chloride | 118.1093 | 3.34 | 0.00     | 159195 | 84.0 | 68.4   | 36.9  | 96.9  |
|                    |          |      |          |        | 86.0 | 44.6   | 14.3  | 74.3  |




# Quantitation Results Report (QT Reviewed)


| Compound                 | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------------|----------|------|----------|--------|------|--------|-------|-------|
| trans-1,2-Dichloroethene | 129.8320 | 3.72 | 0.00     | 121109 | 61.0 | 158.2  | 123.9 | 183.9 |
|                          |          |      |          |        | 98.0 | 62.8   | 35.7  | 95.7  |

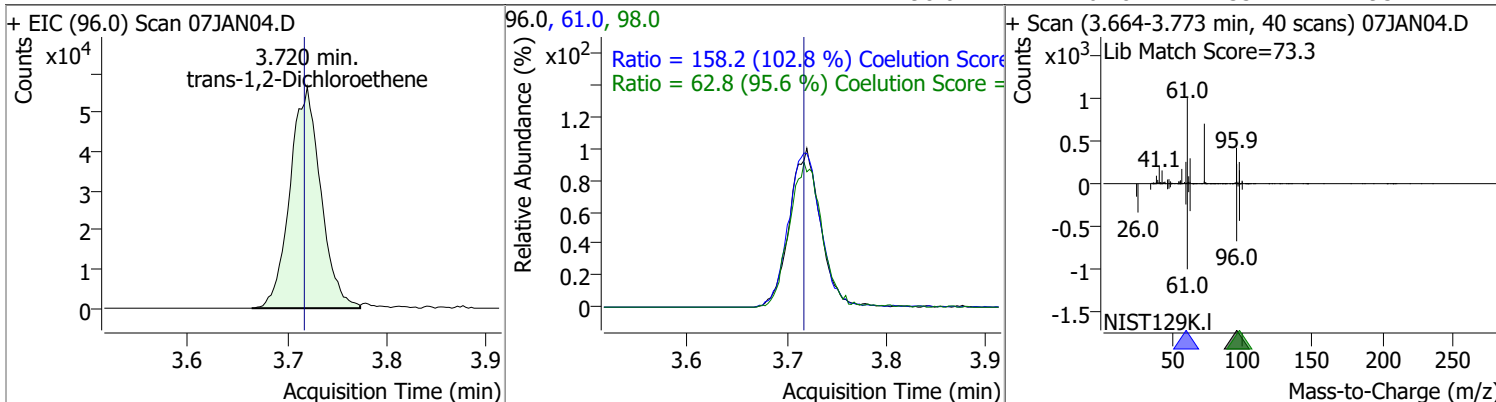

| Compound                       | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------------------|----------|------|----------|--------|------|--------|-------|-------|
| Methyl tert-butyl ether (MTBE) | 132.8050 | 3.76 | 0.00     | 160126 | 57.0 | 25.0   | 0.0   | 54.6  |




| Compound           | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1-Dichloroethane | 131.0789 | 4.38 | 0.00     | 227596 | 65.0 | 32.1   | 2.1   | 62.1  |
|                    |          |      |          |        | 83.0 | 13.5   | 0.0   | 43.7  |




# Quantitation Results Report (QT Reviewed)


| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 2,2-Dichloropropane | 128.7744 | 5.19 | 0.00     | 167542 | 41.0 | 66.5   | 36.5  | 96.5  |
|                     |          |      |          |        | 97.0 | 23.7   | 0.0   | 53.2  |

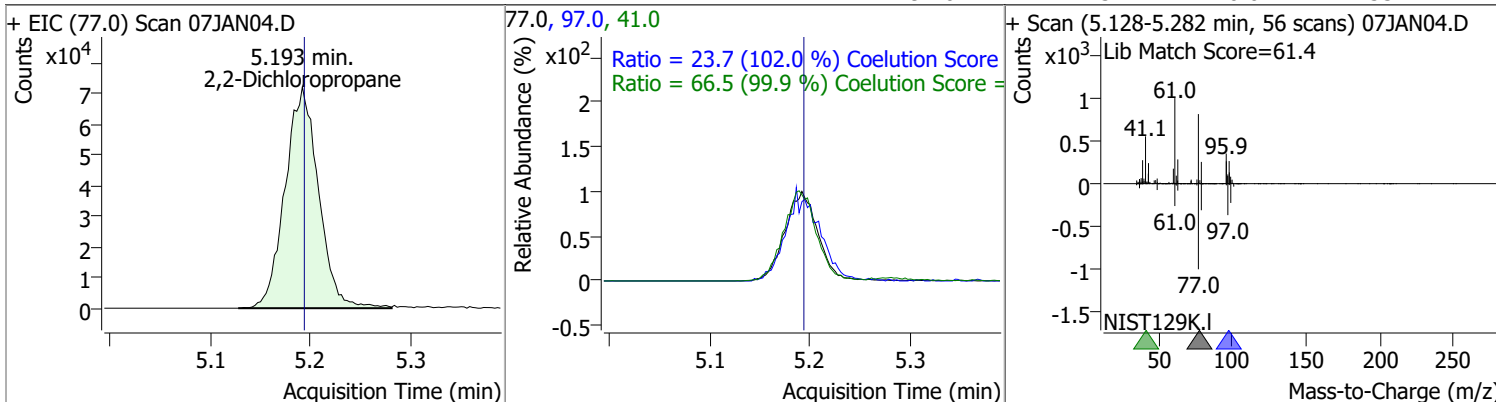


| Compound               | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,2-Dichloroethene | 129.6836 | 5.22 | 0.00     | 122647 | 61.0 | 164.5  | 137.2 | 197.2 |
|                        |          |      |          |        | 98.0 | 65.2   | 37.3  | 97.3  |

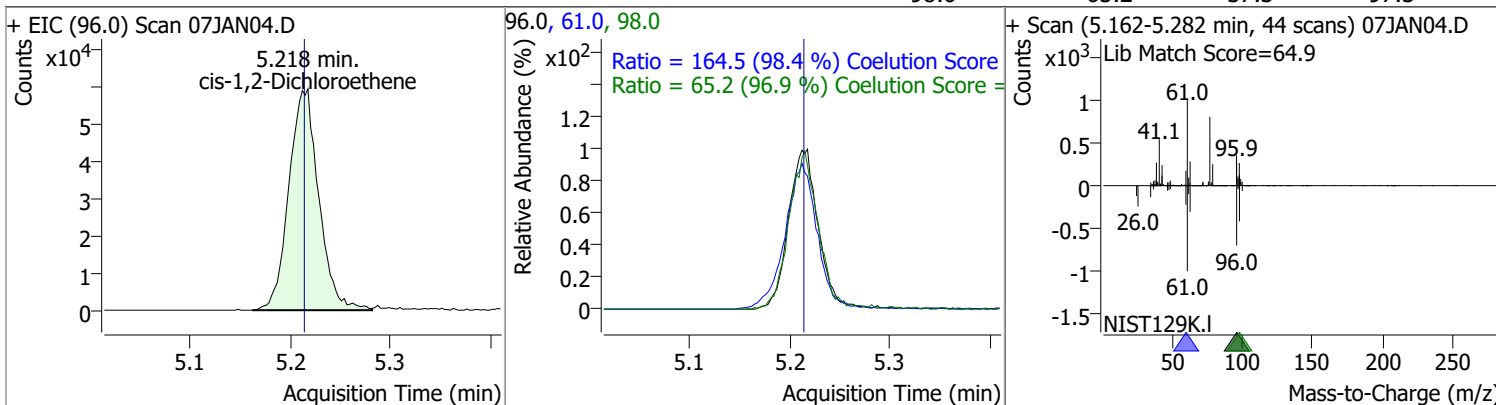





| Compound            | Conc.     | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|-----------|------|----------|--------|------|--------|-------|-------|
| Methyl ethyl ketone | 1138.3128 | 5.28 | 0.00     | 145822 | 72.0 | 22.3   | 0.0   | 51.3  |
|                     |           |      |          |        |      |        |       |       |

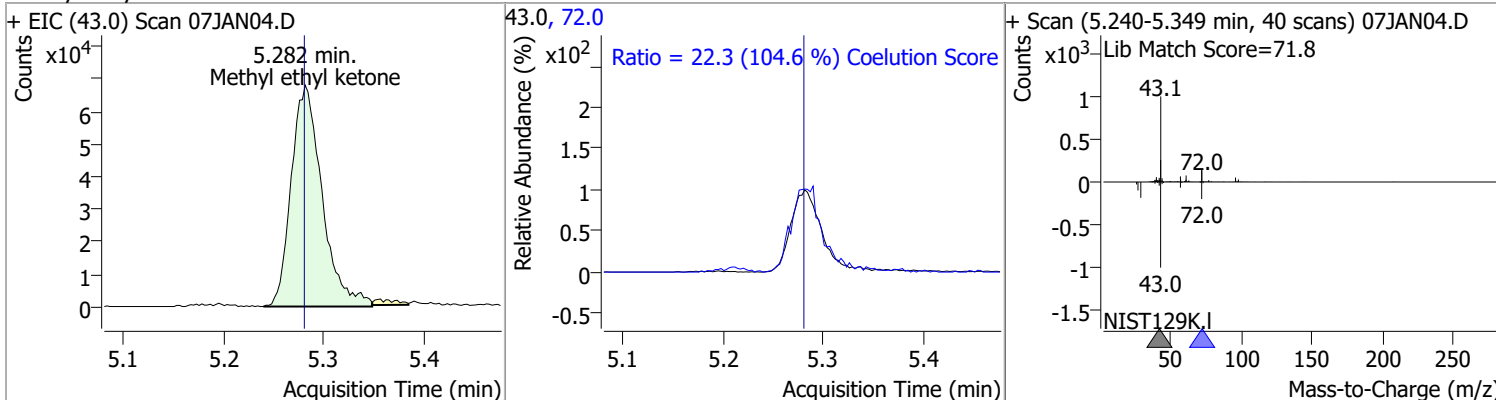

| Compound           | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|-------|------|--------|-------|-------|
| Bromochloromethane | 120.1958 | 5.52 | 0.00     | 47092 | 49.0 | 192.9  | 152.9 | 212.9 |
|                    |          |      |          |       |      |        |       |       |

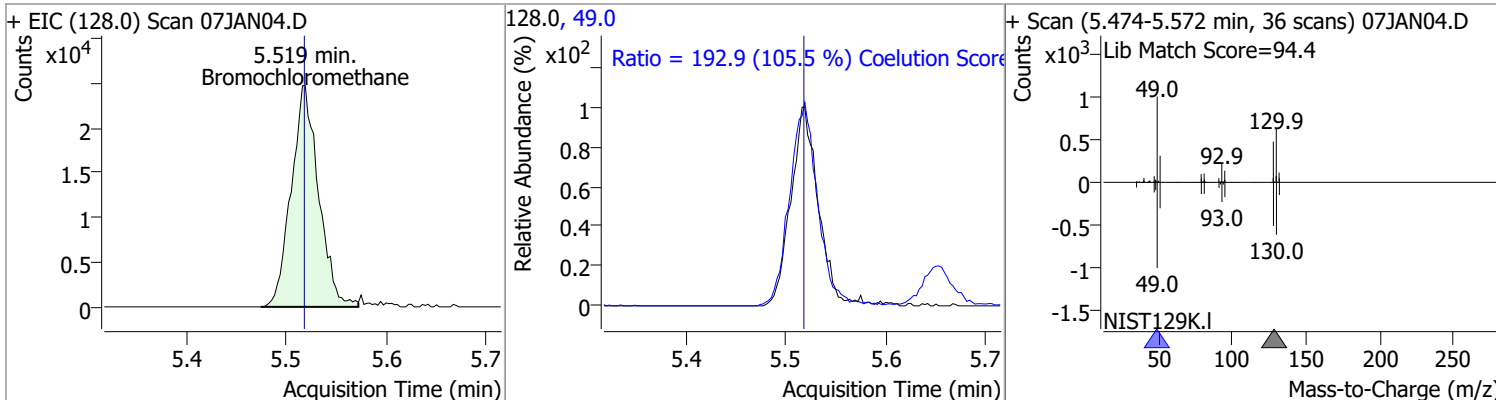


# Quantitation Results Report (QT Reviewed)

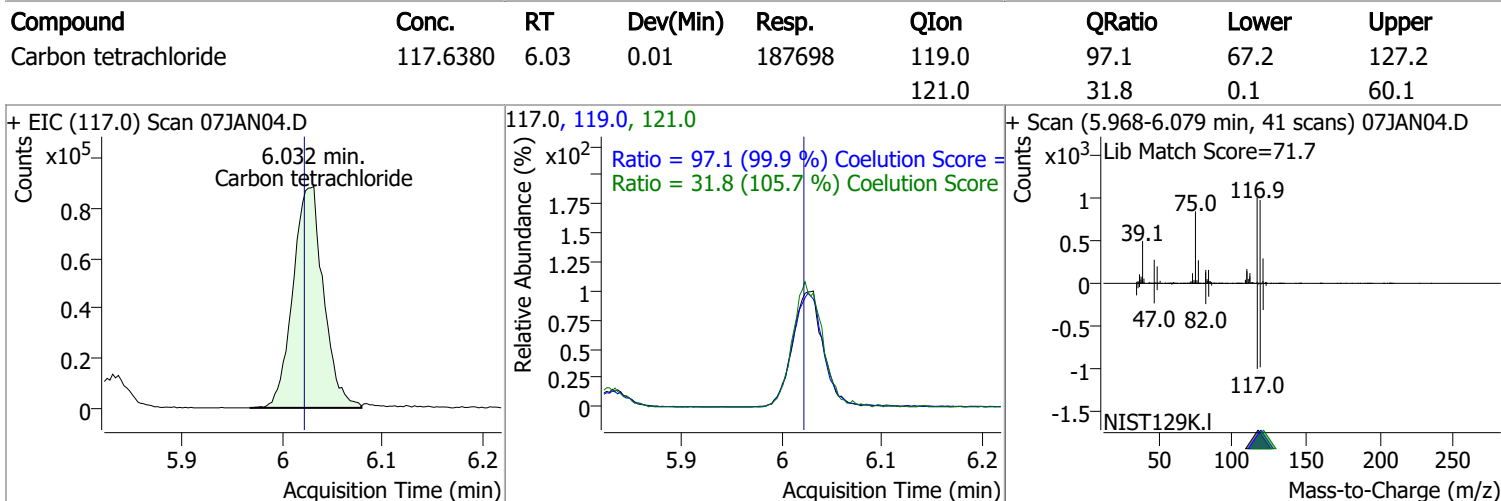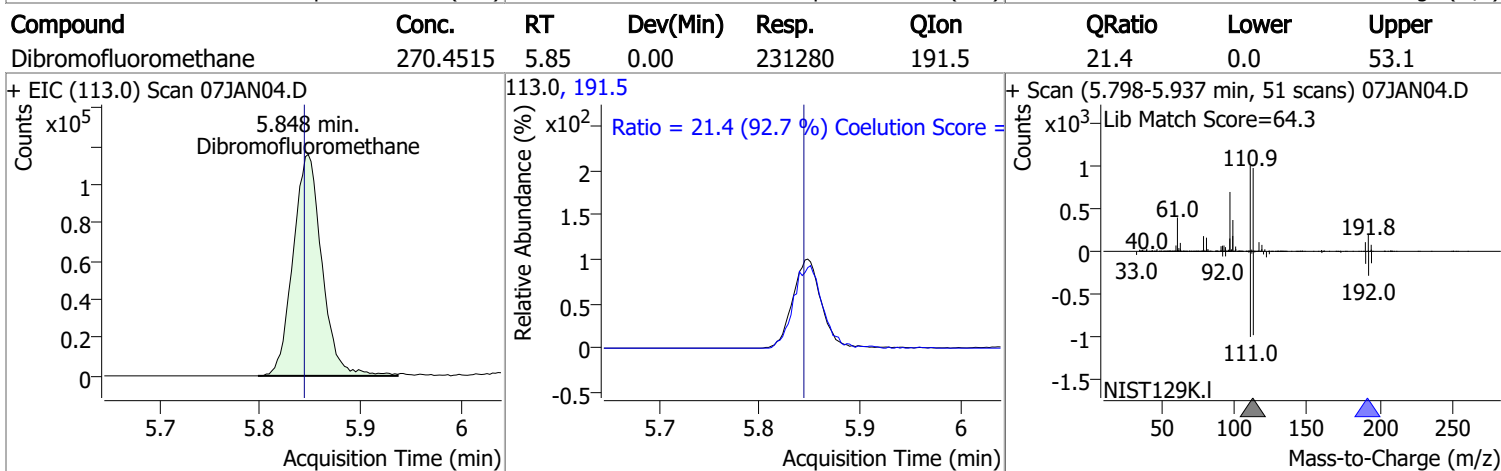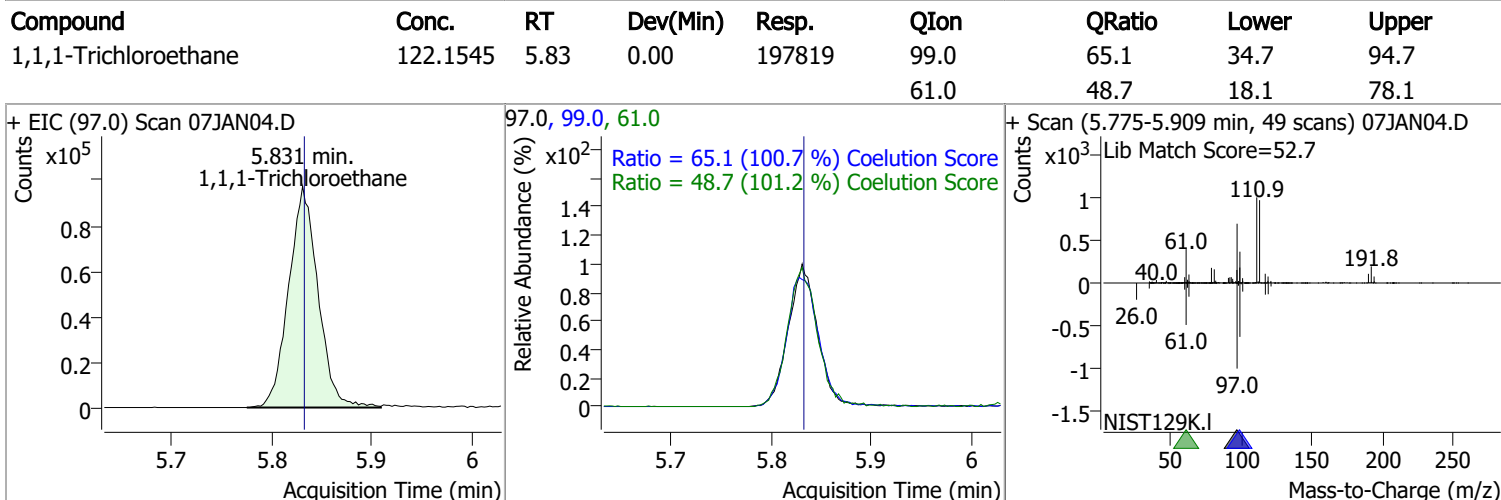


# Quantitation Results Report (QT Reviewed)


| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|-------|--------|-------|-------|
| 1,1-Dichloropropene | 118.0827 | 6.04 | 0.00     | 162591 | 110.0 | 36.1   | 5.9   | 65.9  |
|                     |          |      |          |        | 77.0  | 31.6   | 0.1   | 60.1  |




| Compound              | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 282.9153 | 6.23 | 0.00     | 104500 | 65.0 | 191.1  | 166.5 | 226.5 |



| Compound | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|----------|----------|------|----------|--------|------|--------|-------|-------|
| Benzene  | 127.6093 | 6.28 | 0.00     | 461197 | 77.0 | 23.7   | 0.0   | 53.5  |




| Compound           | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloroethane | 121.9792 | 6.32 | 0.00     | 119261 | 64.0 | 29.8   | 0.0   | 59.9  |
|                    |          |      |          |        | 98.0 | 8.0    | 0.0   | 37.6  |




# Quantitation Results Report (QT Reviewed)


| Compound        | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|-----------------|----------|------|----------|--------|-------|--------|-------|-------|
| Trichloroethene | 125.8989 | 7.03 | 0.00     | 131597 | 130.0 | 100.6  | 71.5  | 131.5 |
|                 |          |      |          |        | 97.0  | 64.3   | 34.1  | 94.1  |

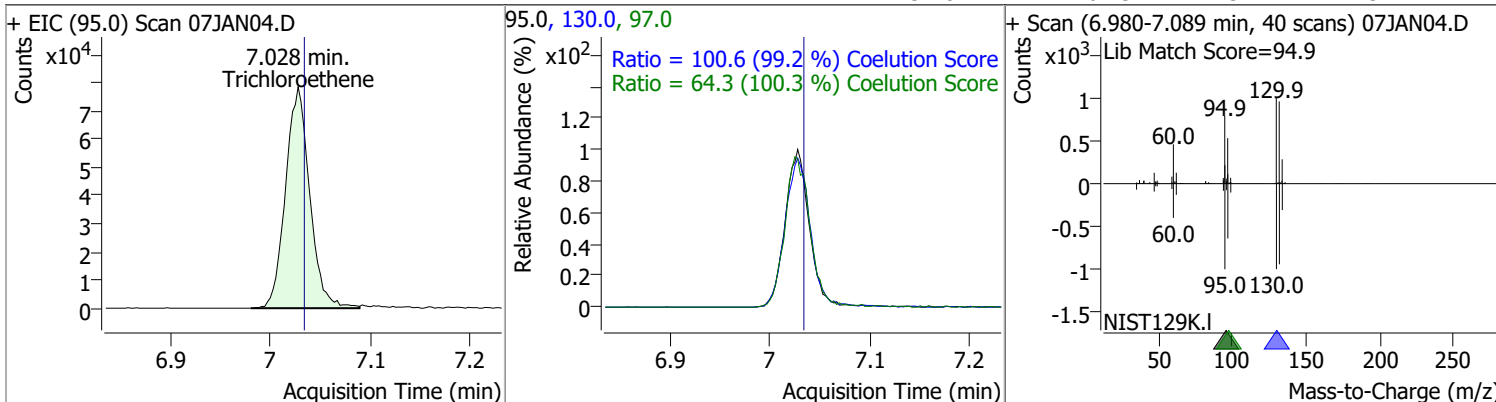

| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloropropane | 124.0744 | 7.27 | 0.00     | 114080 | 76.0 | 38.7   | 8.2   | 68.2  |

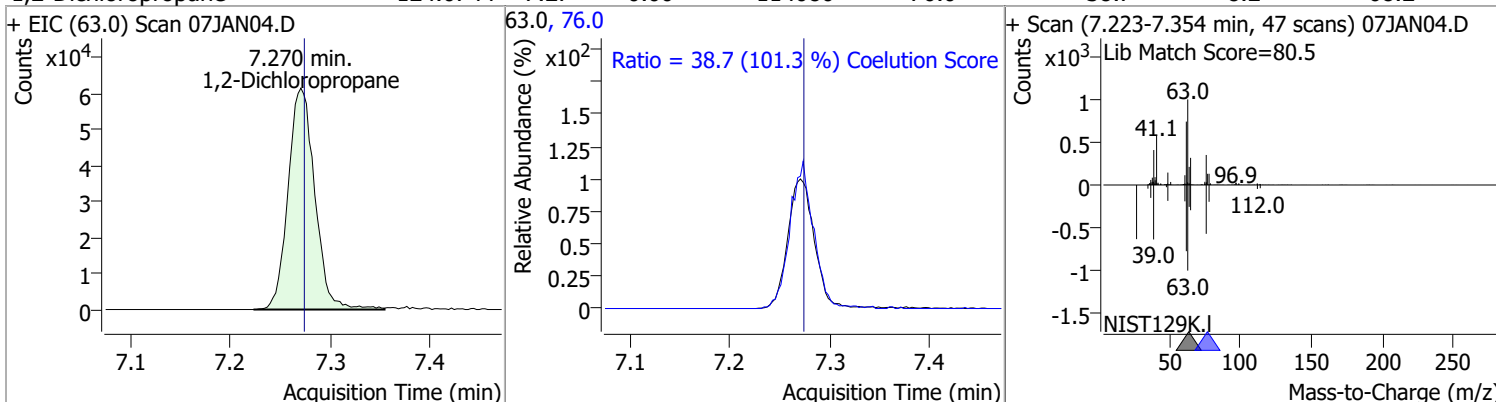


| Compound       | Conc.    | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|----------------|----------|------|----------|-------|-------|--------|-------|-------|
| Dibromomethane | 124.1493 | 7.40 | 0.00     | 48238 | 173.5 | 107.7  | 83.7  | 143.7 |
|                |          |      |          |       | 95.0  | 82.7   | 52.2  | 112.2 |

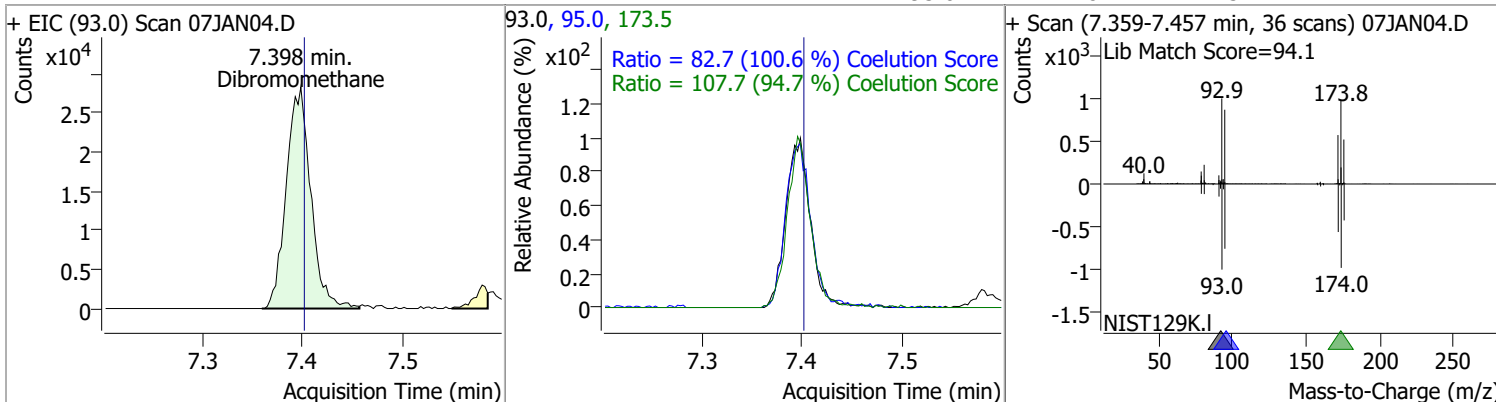




# Quantitation Results Report (QT Reviewed)


| Compound             | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Bromodichloromethane | 127.5739 | 7.58 | 0.00     | 136799 | 85.0  | 63.6   | 34.5  | 94.5  |
|                      |          |      |          |        | 127.0 | 10.0   | 0.0   | 39.6  |

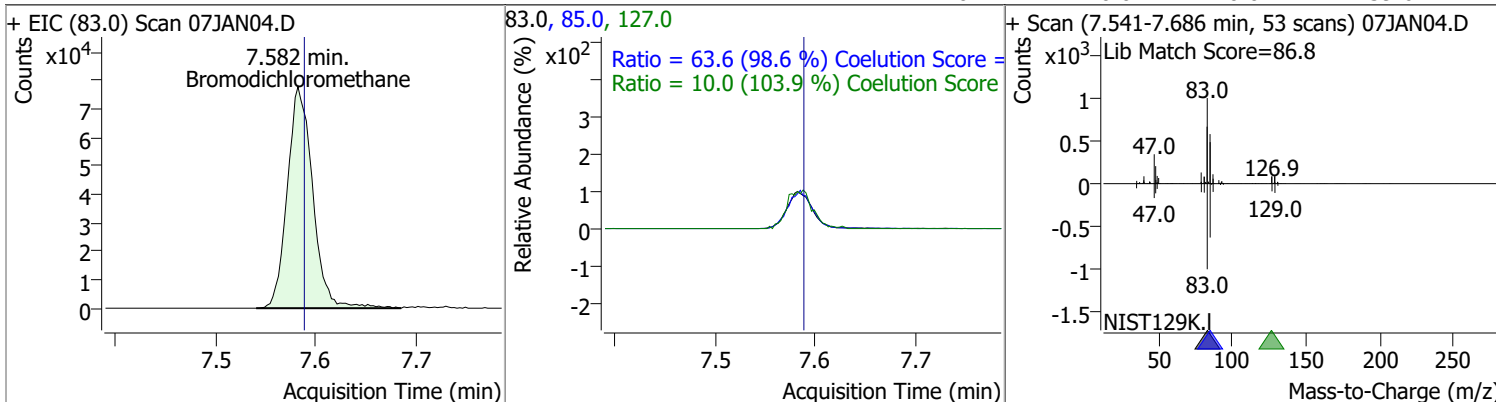

| Compound                | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|-------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,3-Dichloropropene | 117.2568 | 8.06 | 0.00     | 142161 | 39.0 | 54.3   | 23.3  | 83.3  |
|                         |          |      |          |        | 77.0 | 31.1   | 1.0   | 61.0  |

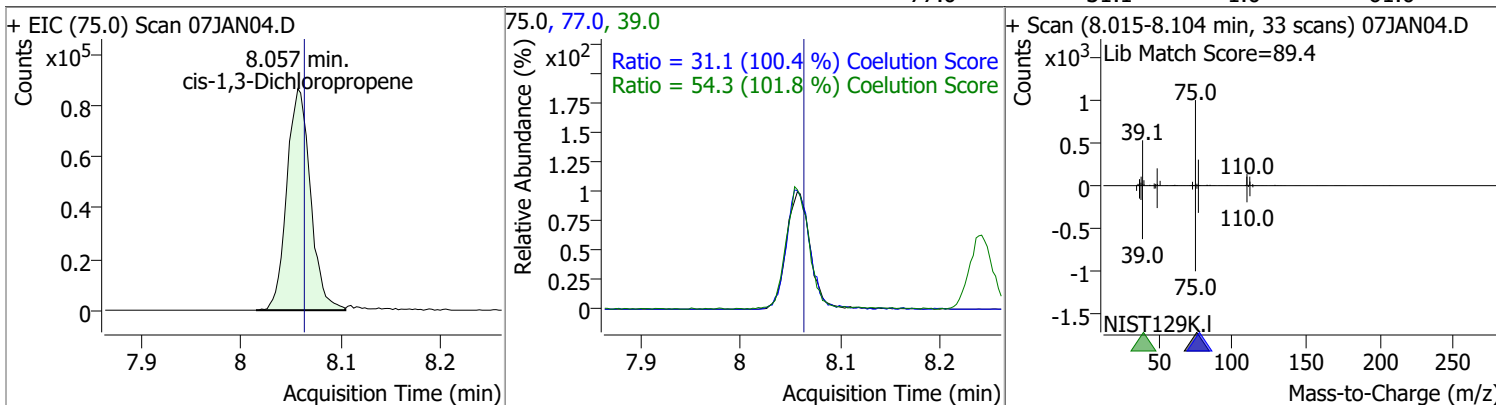


| Compound   | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 271.0520 | 8.32 | 0.00     | 905281 | 100.0 | 64.3   | 34.4  | 94.4  |
|            |          |      |          |        | 99.0  | 9.6    | 0.0   | 39.6  |

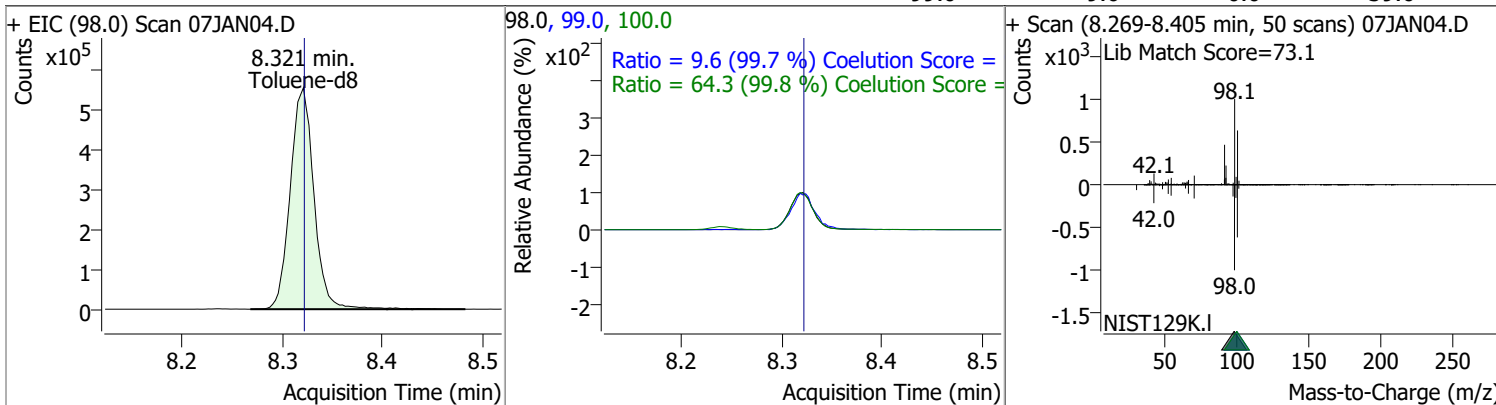


# Quantitation Results Report (QT Reviewed)


| Compound | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|----------|----------|------|----------|--------|------|--------|-------|-------|
| Toluene  | 129.1519 | 8.39 | 0.00     | 291378 | 91.0 | 174.4  | 145.8 | 205.8 |

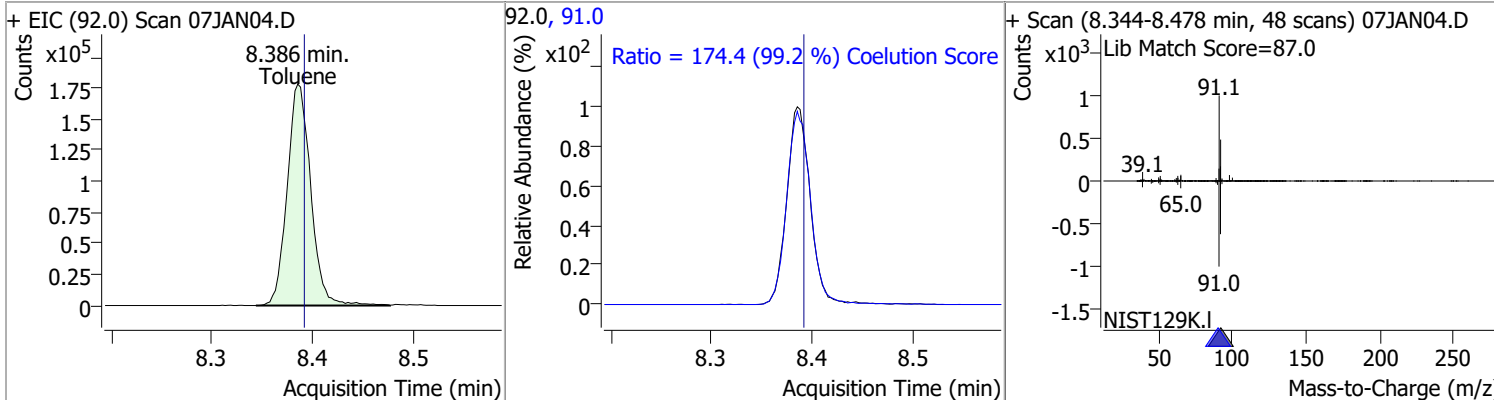

| Compound                  | Conc.    | RT   | Dev(Min) | Resp.  | QIon         | QRatio       | Lower       | Upper        |
|---------------------------|----------|------|----------|--------|--------------|--------------|-------------|--------------|
| trans-1,3-Dichloropropene | 131.2571 | 8.64 | 0.00     | 113275 | 39.0<br>77.0 | 49.1<br>30.9 | 23.4<br>2.4 | 83.4<br>62.4 |




| Compound              | Conc.    | RT   | Dev(Min) | Resp. | QIon         | QRatio        | Lower        | Upper         |
|-----------------------|----------|------|----------|-------|--------------|---------------|--------------|---------------|
| 1,1,2-Trichloroethane | 125.1597 | 8.82 | 0.00     | 56261 | 97.0<br>85.0 | 114.4<br>65.0 | 84.6<br>37.6 | 144.6<br>97.6 |

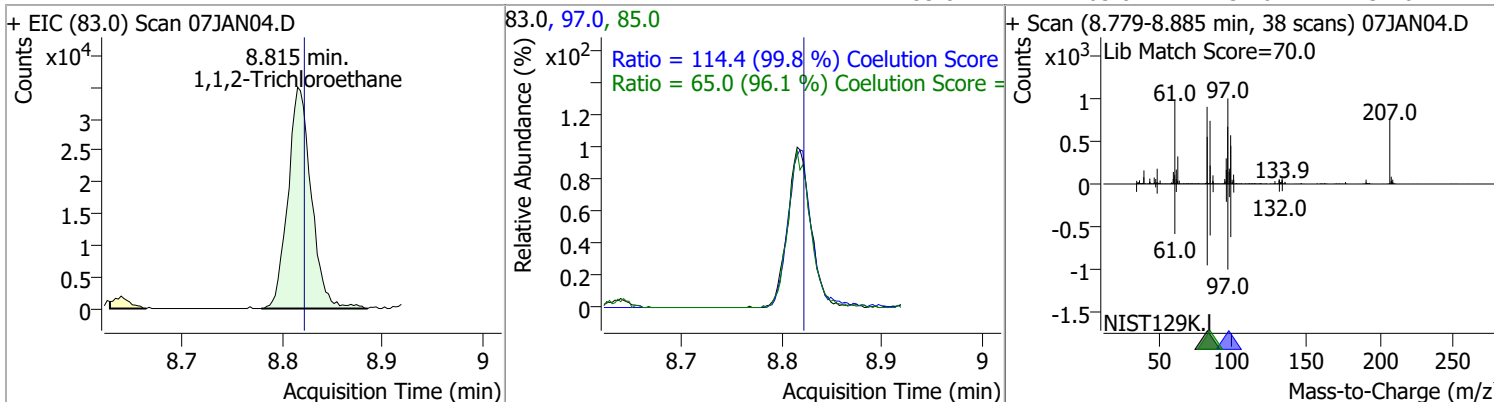


# Quantitation Results Report (QT Reviewed)


| Compound          | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|-------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Tetrachloroethene | 118.8837 | 8.93 | 0.00     | 109421 | 165.8 | 128.1  | 98.6  | 158.6 |
|                   |          |      |          |        | 129.0 | 91.3   | 61.5  | 121.5 |




| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,3-Dichloropropane | 121.3850 | 8.98 | 0.00     | 107326 | 78.0 | 32.3   | 2.9   | 62.9  |















| Compound             | Conc.    | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|----------------------|----------|------|----------|-------|-------|--------|-------|-------|
| Chlorodibromomethane | 122.7318 | 9.21 | 0.00     | 86224 | 127.0 | 77.0   | 48.0  | 108.0 |



| Compound          | Conc.    | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|-------------------|----------|------|----------|-------|-------|--------|-------|-------|
| 1,2-Dibromoethane | 123.1519 | 9.31 | 0.00     | 60530 | 109.0 | 94.3   | 64.5  | 124.5 |




# Quantitation Results Report (QT Reviewed)

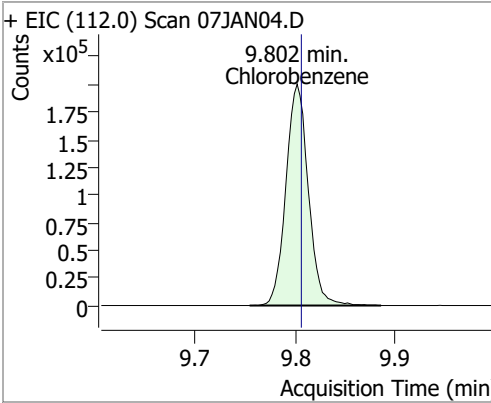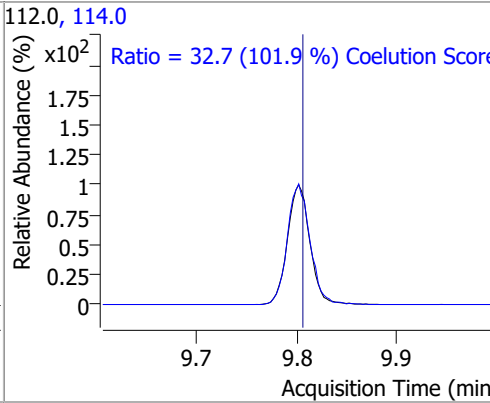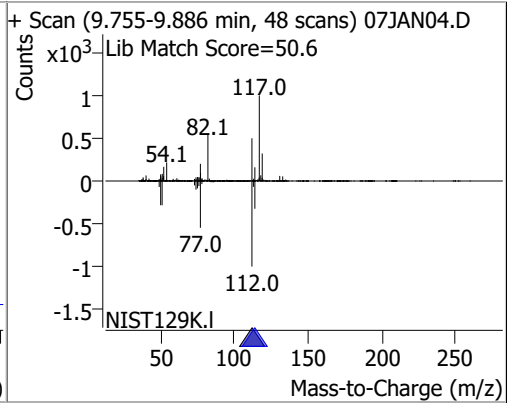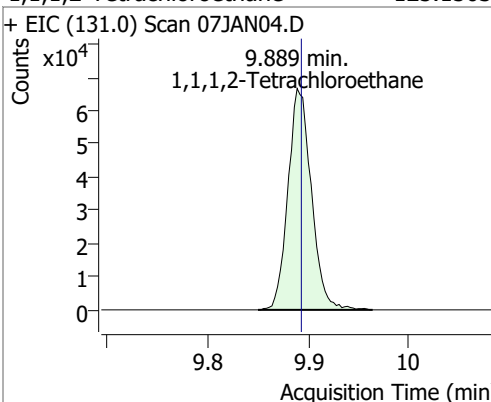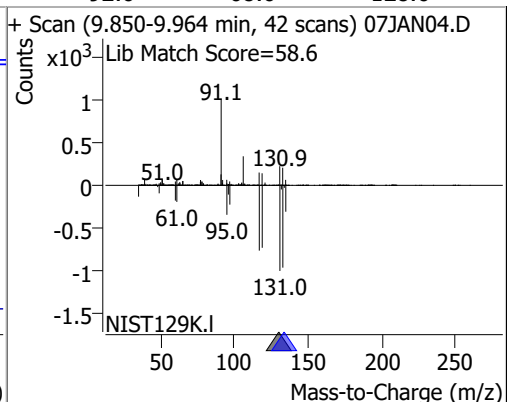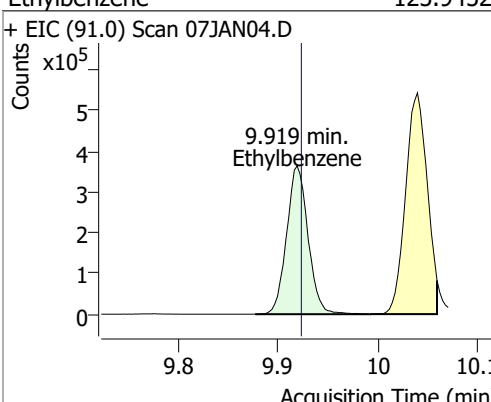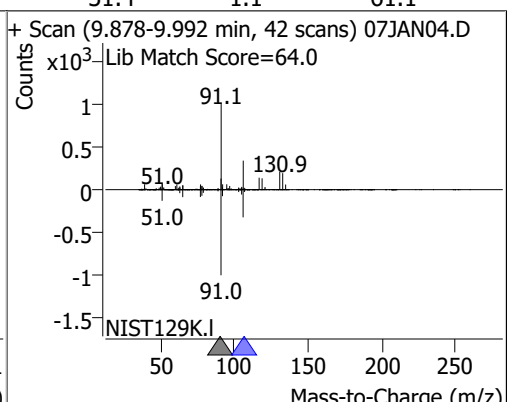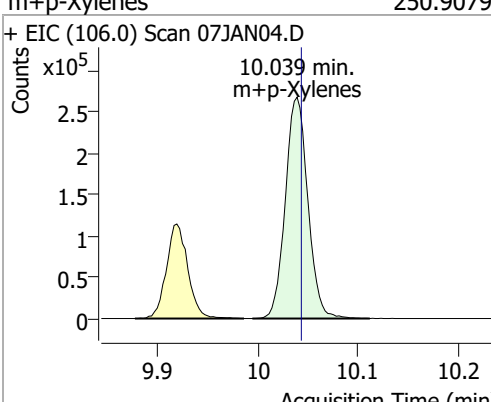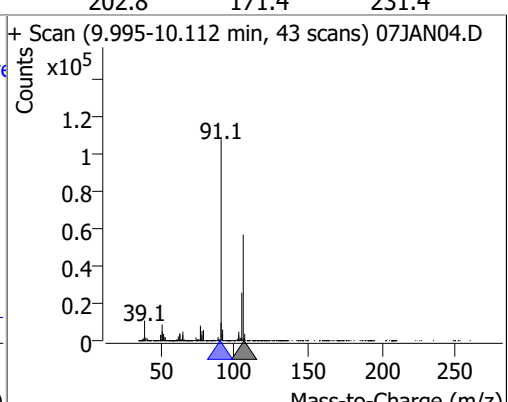
| Compound                                                                                                           | Conc.    | RT    | Dev(Min)                                                                                                                                       | Resp.  | QIon  | QRatio                                                                                                                                                        | Lower | Upper |
|--------------------------------------------------------------------------------------------------------------------|----------|-------|------------------------------------------------------------------------------------------------------------------------------------------------|--------|-------|---------------------------------------------------------------------------------------------------------------------------------------------------------------|-------|-------|
| Chlorobenzene                                                                                                      | 125.6477 | 9.80  | 0.00                                                                                                                                           | 310348 | 114.0 | 32.7                                                                                                                                                          | 2.1   | 62.1  |
| + EIC (112.0) Scan 07JAN04.D<br>   |          |       | 112.0, 114.0<br>Ratio = 32.7 (101.9 %) Coelution Score<br>   |        |       | + Scan (9.755-9.886 min, 48 scans) 07JAN04.D<br>Lib Match Score=50.6<br>   |       |       |
| 1,1,1,2-Tetrachloroethane                                                                                          | 125.1503 | 9.89  | 0.00                                                                                                                                           | 108057 | 133.0 | 92.6                                                                                                                                                          | 68.6  | 128.6 |
| + EIC (131.0) Scan 07JAN04.D<br>  |          |       | 131.0, 133.0<br>Ratio = 92.6 (93.9 %) Coelution Score<br>   |        |       | + Scan (9.850-9.964 min, 42 scans) 07JAN04.D<br>Lib Match Score=58.6<br>  |       |       |
| Ethylbenzene                                                                                                       | 125.9452 | 9.92  | 0.00                                                                                                                                           | 539522 | 106.0 | 31.4                                                                                                                                                          | 1.1   | 61.1  |
| + EIC (91.0) Scan 07JAN04.D<br>  |          |       | 91.0, 106.0<br>Ratio = 31.4 (101.0 %) Coelution Score<br>  |        |       | + Scan (9.878-9.992 min, 42 scans) 07JAN04.D<br>Lib Match Score=64.0<br> |       |       |
| m+p-Xylenes                                                                                                        | 250.9079 | 10.04 | 0.00                                                                                                                                           | 417695 | 91.0  | 202.8                                                                                                                                                         | 171.4 | 231.4 |
| + EIC (106.0) Scan 07JAN04.D<br> |          |       | 106.0, 91.0<br>Ratio = 202.8 (100.7 %) Coelution Score<br> |        |       | + Scan (9.995-10.112 min, 43 scans) 07JAN04.D<br>                        |       |       |

# Quantitation Results Report (QT Reviewed)


| Compound | Conc.    | RT    | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|----------|----------|-------|----------|--------|------|--------|-------|-------|
| o-Xylene | 129.8994 | 10.43 | 0.00     | 192510 | 91.0 | 212.9  | 183.1 | 243.1 |

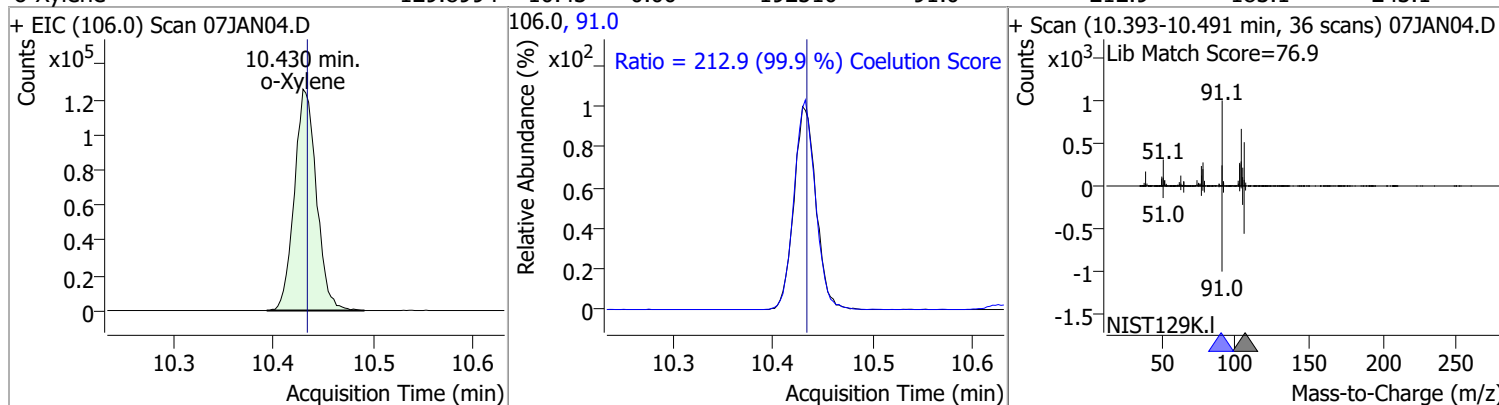


| Compound | Conc.    | RT    | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|----------|----------|-------|----------|--------|------|--------|-------|-------|
| Styrene  | 132.5150 | 10.45 | 0.00     | 316187 | 78.0 | 49.4   | 19.6  | 79.6  |

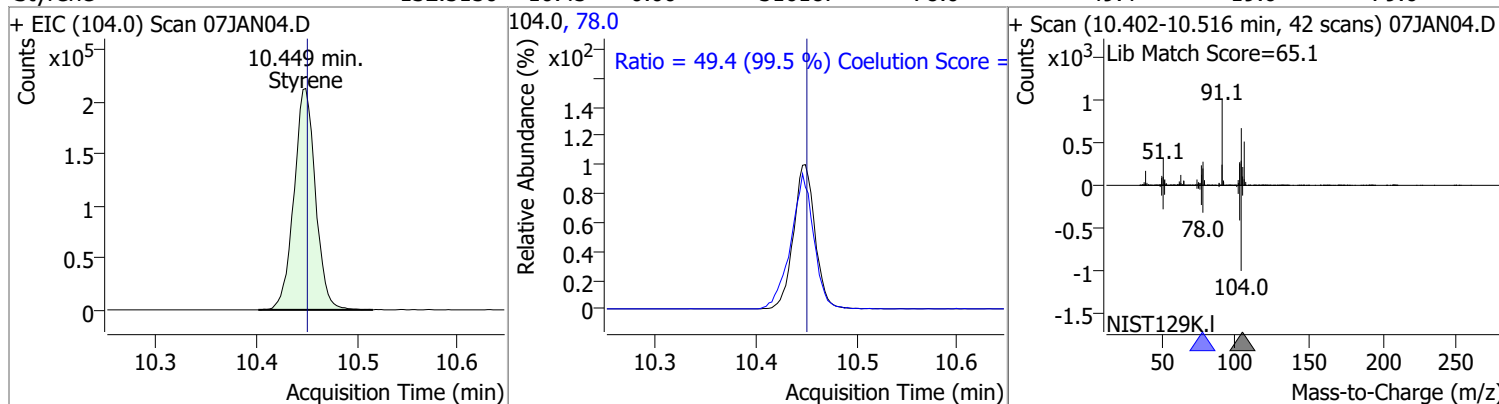

| Compound  | Conc.    | RT    | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|-----------|----------|-------|----------|-------|-------|--------|-------|-------|
| Bromoform | 131.1556 | 10.62 | 0.00     | 47153 | 170.5 | 51.7   | 22.1  | 82.1  |
|           |          |       |          |       | 174.5 | 49.5   | 20.1  | 80.1  |

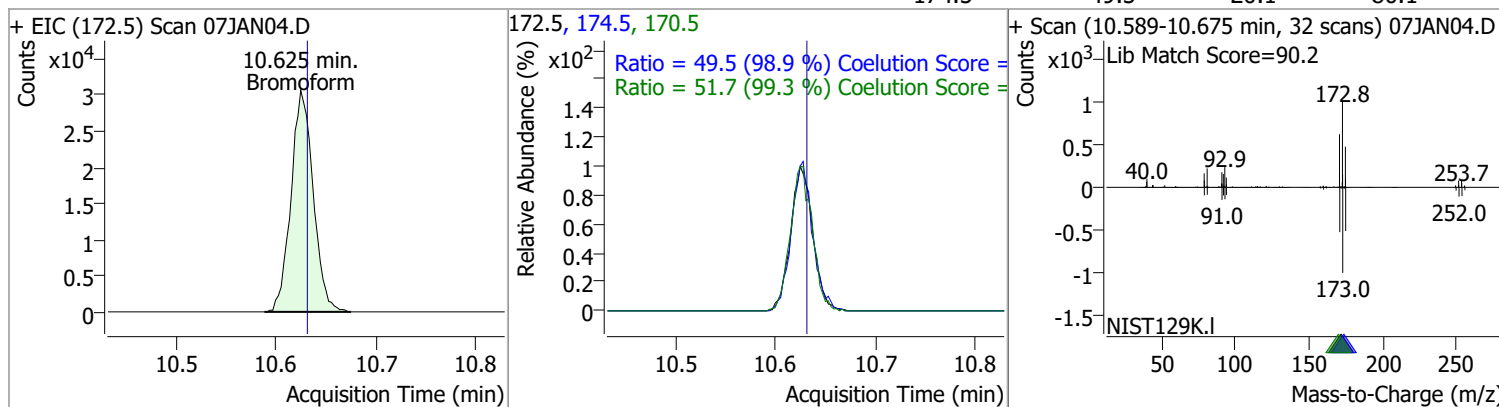


| Compound             | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 271.9817 | 10.95 | 0.00     | 279940 | 174.0 | 91.9   | 61.7  | 121.7 |
|                      |          |       |          |        | 176.0 | 90.9   | 60.6  | 120.6 |

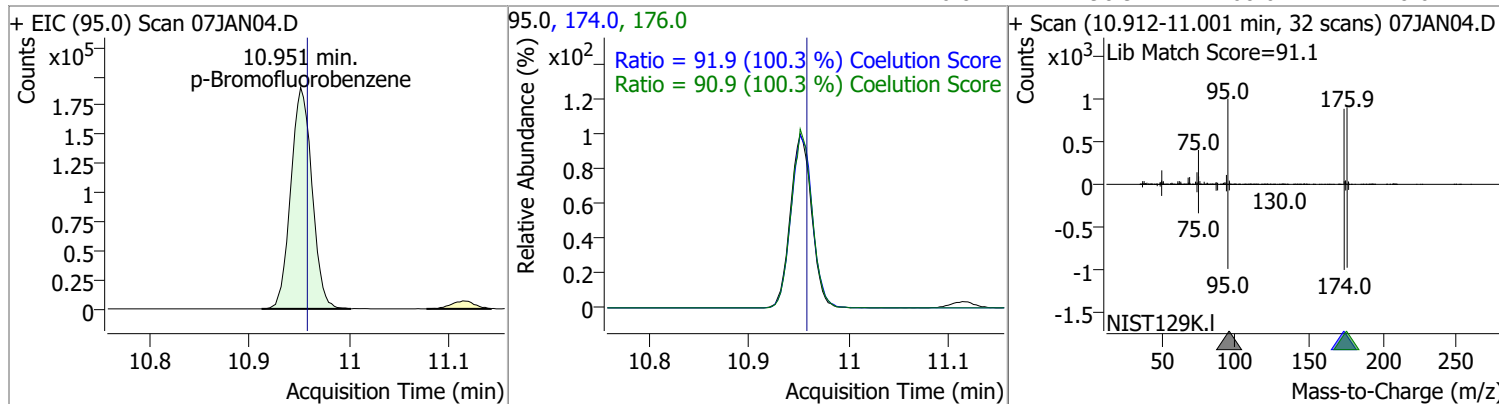


# Quantitation Results Report (QT Reviewed)


| Compound     | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|--------------|----------|-------|----------|--------|-------|--------|-------|-------|
| Bromobenzene | 131.5649 | 11.09 | 0.00     | 119622 | 77.0  | 145.2  | 115.7 | 175.7 |
|              |          |       |          |        | 158.0 | 96.4   | 66.5  | 126.5 |




| Compound                  | Conc.    | RT    | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|----------|-------|----------|-------|------|--------|-------|-------|
| 1,1,2,2-Tetrachloroethane | 123.1192 | 11.11 | -0.01    | 64431 | 85.0 | 67.5   | 36.2  | 96.2  |

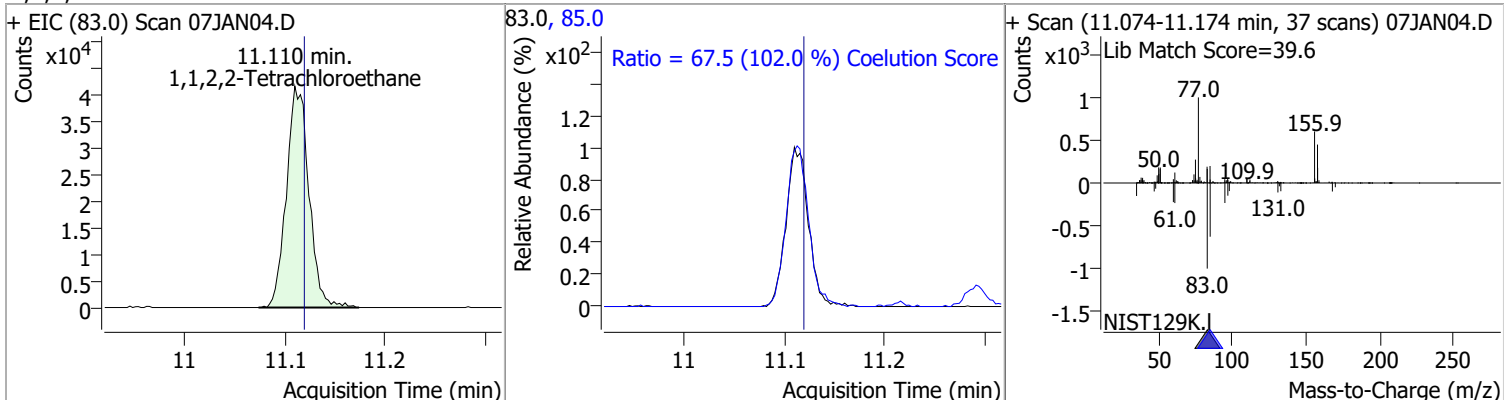

| Compound               | Conc.    | RT    | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|------------------------|----------|-------|----------|-------|-------|--------|-------|-------|
| 1,2,3-Trichloropropane | 125.1764 | 11.15 | 0.00     | 17528 | 112.0 | 64.2   | 33.5  | 93.5  |






| Compound        | Conc.    | RT    | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|-----------------|----------|-------|----------|--------|------|--------|-------|-------|
| 2-Chlorotoluene | 130.0465 | 11.29 | 0.00     | 117650 | 91.0 | 288.8  | 252.3 | 312.3 |






# Quantitation Results Report (QT Reviewed)




| Compound        | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|-----------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 4-Chlorotoluene | 134.9812 | 11.40 | 0.00     | 398147 | 126.0 | 31.6   | 1.7   | 61.7  |



|                     |          |       |      |        |       |      |      |      |
|---------------------|----------|-------|------|--------|-------|------|------|------|
| 1,3-Dichlorobenzene | 131.9494 | 12.04 | 0.01 | 218804 | 148.0 | 63.1 | 33.6 | 93.6 |
|                     |          |       |      |        | 111.0 | 39.0 | 9.8  | 69.8 |






|                     |          |       |      |        |       |      |      |      |
|---------------------|----------|-------|------|--------|-------|------|------|------|
| 1,4-Dichlorobenzene | 128.6355 | 12.13 | 0.00 | 217500 | 148.0 | 63.8 | 33.1 | 93.1 |
|                     |          |       |      |        | 111.0 | 39.0 | 9.1  | 69.1 |



# Quantitation Results Report (QT Reviewed)


| Compound            | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,2-Dichlorobenzene | 125.5596 | 12.49 | 0.00     | 175961 | 148.0 | 63.9   | 33.9  | 93.9  |
|                     |          |       |          |        | 111.0 | 39.9   | 11.0  | 71.0  |





# Quantitation Results Report (QT Reviewed)

|                |                                     |                   |                       |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File      | 07JAN06.D                           | Operator          | MSC                   |
| Acq. Method    | 5975CACQF.M                         | Acq. Date-Time    | 1/7/2022 11:45:07 AM  |
| Sample Name    | MBLK010722_                         | Instrument        | VOA5975C              |
| Vial           | 6                                   | Multiplier        | 1.00                  |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m  | Comment           |                       |
| Tune File      | BFB_Atune3.u                        | Tune Date         | 10/11/2021 4:02:00 PM |
| Batch Name     | VG010722_8260B.batch.bin            | Last Calib Update | 3/2/2022 10:41:44 AM  |
| Ref Library    | \\MASSHUNTER\Org\Library\NIST129K.I |                   |                       |

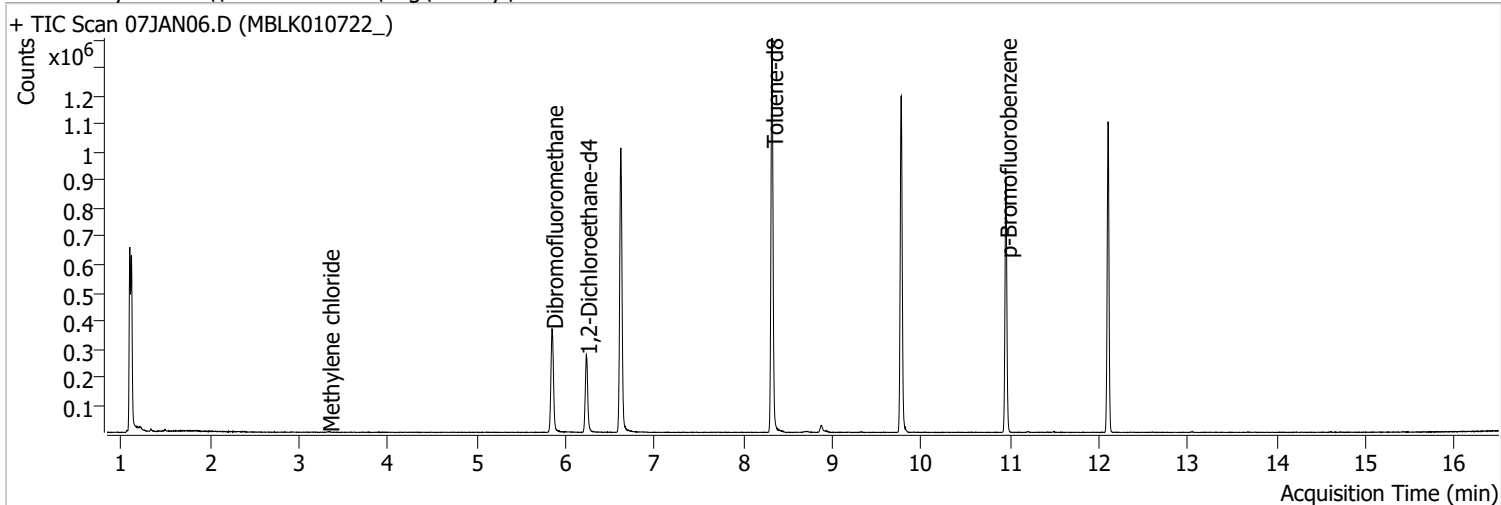









| Compound                           | RT                   | QIon  | Resp.  | Conc.              | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|--------------------|-------|----------|
| <b>Internal Standards</b>          |                      |       |        |                    |       |          |
| M Fluorobenzene                    | 6.620                | 96.0  | 869267 | 250.0000           | ng    | -0.003   |
| M Chlorobenzene-d5                 | 9.772                | 82.0  | 339487 | 250.0000           | ng    | 0.000    |
| M 1,4-Dichlorobenzene-d4           | 12.103               | 152.0 | 257432 | 250.0000           | ng    | 0.003    |
| <b>System Monitoring Compounds</b> |                      |       |        |                    |       |          |
| S Dibromofluoromethane             | 5.845                | 113.0 | 221741 | 270.7666           | ng    | 0.000    |
| Spiked Amount: 250.000             | Range: 80.0 - 119.0% |       |        | Recovery = 108.31% |       |          |
| S 1,2-Dichloroethane-d4            | 6.230                | 67.0  | 98740  | 279.1458           | ng    | -0.003   |
| Spiked Amount: 250.000             | Range: 81.0 - 118.0% |       |        | Recovery = 111.66% |       |          |
| S Toluene-d8                       | 8.321                | 98.0  | 864903 | 264.3775           | ng    | 0.003    |
| Spiked Amount: 250.000             | Range: 89.0 - 112.0% |       |        | Recovery = 105.75% |       |          |
| S p-Bromofluorobenzene             | 10.951               | 95.0  | 259344 | 274.9894           | ng    | -0.003   |
| Spiked Amount: 250.000             | Range: 85.0 - 114.0% |       |        | Recovery = 110.00% |       |          |
| <b>Target Compounds</b>            |                      |       |        |                    |       |          |
| T Dichlorodifluoromethane          | 0.000                |       | 0      | N.D.               |       |          |
| T Chloromethane                    | 0.000                |       | 0      | N.D.               |       |          |
| T Vinyl chloride                   | 0.000                |       | 0      | N.D.               |       |          |
| T Bromomethane                     | 0.000                |       | 0      | N.D.               |       |          |
| T Chloroethane                     | 0.000                |       | 0      | N.D.               |       |          |
| T Trichlorofluoromethane           | 0.000                |       | 0      | N.D.               |       |          |
| T 1,1-Dichloroethene               | 0.000                |       | 0      | N.D.               |       |          |
| T Methylene chloride               | 3.330                | 49.0  | 1664   | 1.2889             | ng    | m 84     |
| T trans-1,2-Dichloroethene         | 0.000                |       | 0      | N.D.               |       |          |
| T Methyl tert-butyl ether (MTBE)   | 0.000                |       | 0      | N.D.               |       |          |
| T 1,1-Dichloroethane               | 0.000                |       | 0      | N.D.               |       |          |
| T 2,2-Dichloropropane              | 0.000                |       | 0      | N.D.               |       |          |
| T cis-1,2-Dichloroethene           | 0.000                |       | 0      | N.D.               |       |          |
| T Methyl ethyl ketone              | 0.000                |       | 0      | N.D.               |       |          |
| T Bromochloromethane               | 0.000                |       | 0      | N.D.               |       |          |
| T Chloroform                       | 0.000                |       | 0      | N.D.               |       |          |

# Quantitation Results Report (QT Reviewed)

| Compound                    | RT    | QIon | Resp. | Conc. | Units | Dev(Min) |
|-----------------------------|-------|------|-------|-------|-------|----------|
| T 1,1,1-Trichloroethane     | 0.000 |      | 0     | N.D.  |       |          |
| T Carbon tetrachloride      | 0.000 |      | 0     | N.D.  |       |          |
| T 1,1-Dichloropropene       | 0.000 |      | 0     | N.D.  |       |          |
| T Benzene                   | 0.000 |      | 0     | N.D.  |       |          |
| T 1,2-Dichloroethane        | 0.000 |      | 0     | N.D.  |       |          |
| T Trichloroethene           | 0.000 |      | 0     | N.D.  |       |          |
| T 1,2-Dichloropropane       | 0.000 |      | 0     | N.D.  |       |          |
| T Dibromomethane            | 0.000 |      | 0     | N.D.  |       |          |
| T Bromodichloromethane      | 0.000 |      | 0     | N.D.  |       |          |
| T cis-1,3-Dichloropropene   | 0.000 |      | 0     | N.D.  |       |          |
| T Toluene                   | 0.000 |      | 0     | N.D.  |       |          |
| T trans-1,3-Dichloropropene | 0.000 |      | 0     | N.D.  |       |          |
| T 1,1,2-Trichloroethane     | 0.000 |      | 0     | N.D.  |       |          |
| T Tetrachloroethene         | 0.000 |      | 0     | N.D.  |       |          |
| T 1,3-Dichloropropane       | 0.000 |      | 0     | N.D.  |       |          |
| T Chlorodibromomethane      | 0.000 |      | 0     | N.D.  |       |          |
| T 1,2-Dibromoethane         | 0.000 |      | 0     | N.D.  |       |          |
| T Chlorobenzene             | 0.000 |      | 0     | N.D.  |       |          |
| T 1,1,1,2-Tetrachloroethane | 0.000 |      | 0     | N.D.  |       |          |
| T Ethylbenzene              | 0.000 |      | 0     | N.D.  |       |          |
| T m+p-Xylenes               | 0.000 |      | 0     | N.D.  |       |          |
| T o-Xylene                  | 0.000 |      | 0     | N.D.  |       |          |
| T Styrene                   | 0.000 |      | 0     | N.D.  |       |          |
| T Bromoform                 | 0.000 |      | 0     | N.D.  |       |          |
| T Bromobenzene              | 0.000 |      | 0     | N.D.  |       |          |
| T 1,1,2,2-Tetrachloroethane | 0.000 |      | 0     | N.D.  |       |          |
| T 1,2,3-Trichloropropane    | 0.000 |      | 0     | N.D.  |       |          |
| T 2-Chlorotoluene           | 0.000 |      | 0     | N.D.  |       |          |
| T 4-Chlorotoluene           | 0.000 |      | 0     | N.D.  |       |          |
| T 1,3-Dichlorobenzene       | 0.000 |      | 0     | N.D.  |       |          |
| T 1,4-Dichlorobenzene       | 0.000 |      | 0     | N.D.  |       |          |
| T 1,2-Dichlorobenzene       | 0.000 |      | 0     | N.D.  |       |          |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (\*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

# Quantitation Results Report (QT Reviewed)

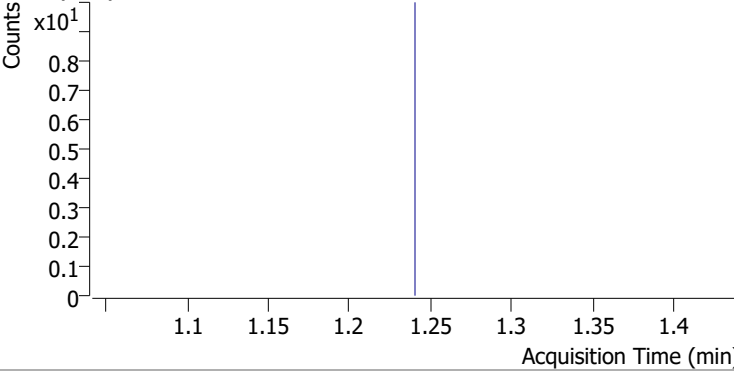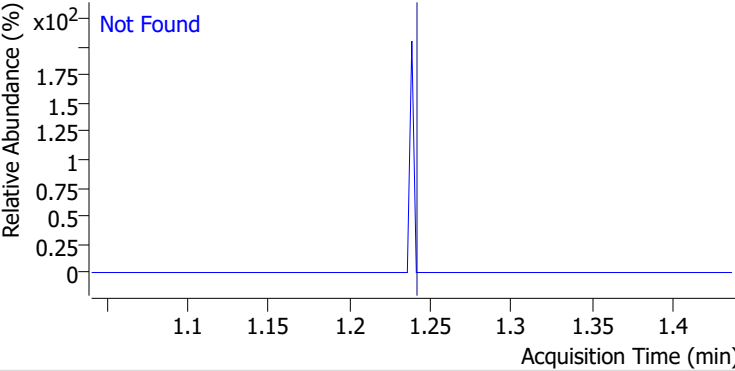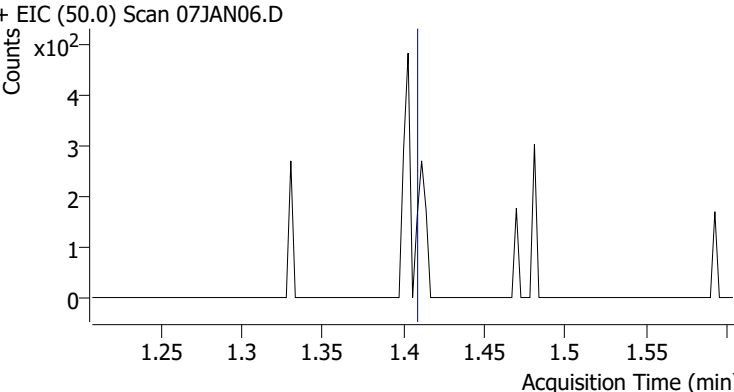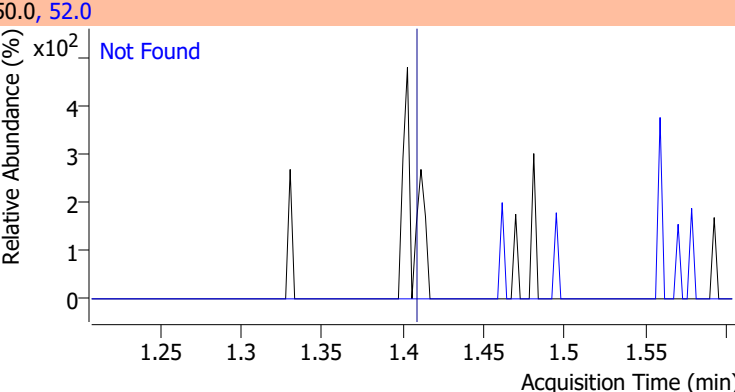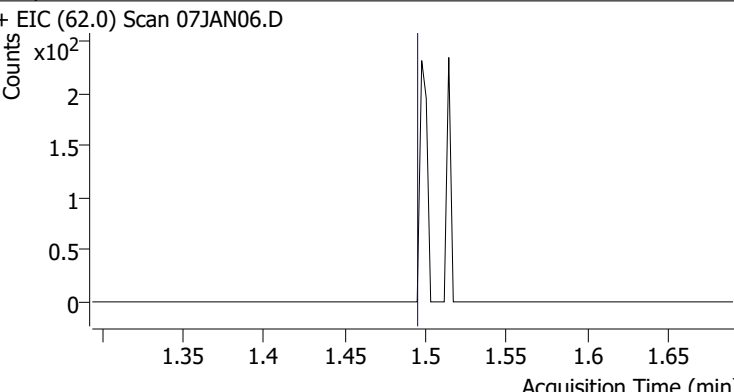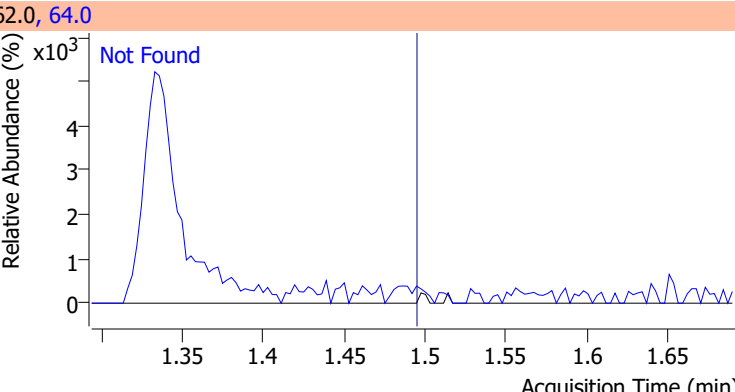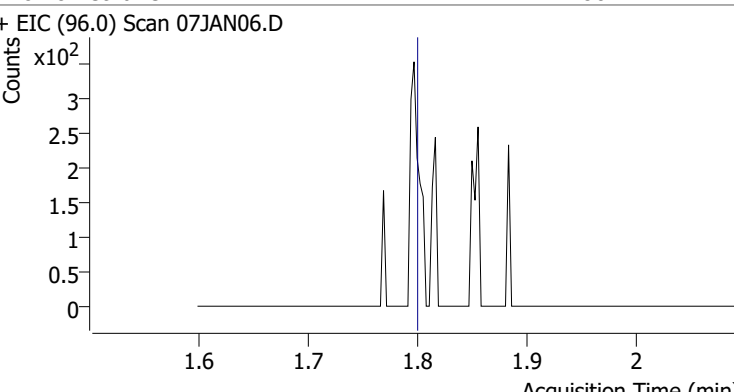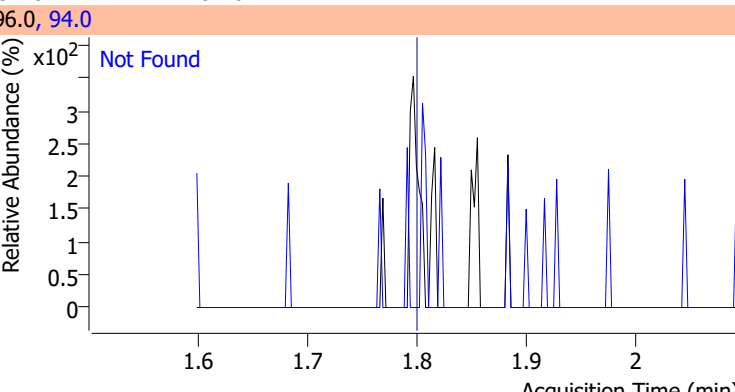
| Compound                                                                           | Conc. | Exp RT | QIon                                                                                 | Exp Ratio |
|------------------------------------------------------------------------------------|-------|--------|--------------------------------------------------------------------------------------|-----------|
| Dichlorodifluoromethane                                                            | N.D.  | 1.24   | 87.0                                                                                 | 32.3      |
| + EIC (85.0) Scan 07JAN06.D ***NO DATA POINTS***                                   |       |        | 85.0, 87.0                                                                           |           |
|    |       |        |    |           |
| Chloromethane                                                                      | N.D.  | 1.41   | 52.0                                                                                 | 32.1      |
| + EIC (50.0) Scan 07JAN06.D                                                        |       |        | 50.0, 52.0                                                                           |           |
|   |       |        |   |           |
| Vinyl chloride                                                                     | N.D.  | 1.50   | 64.0                                                                                 | 29.9      |
| + EIC (62.0) Scan 07JAN06.D                                                        |       |        | 62.0, 64.0                                                                           |           |
|  |       |        |  |           |
| Bromomethane                                                                       | N.D.  | 1.80   | 94.0                                                                                 | 104.6     |
| + EIC (96.0) Scan 07JAN06.D                                                        |       |        | 96.0, 94.0                                                                           |           |
|  |       |        |  |           |

# Quantitation Results Report (QT Reviewed)


| Compound     | Conc. | Exp RT | QIon | Exp Ratio |
|--------------|-------|--------|------|-----------|
| Chloroethane | N.D.  | 1.89   | 66.0 | 30.1      |




| Compound               | Conc. | Exp RT | QIon  | Exp Ratio |
|------------------------|-------|--------|-------|-----------|
| Trichlorofluoromethane | N.D.  | 2.14   | 103.0 | 64.2      |











| Compound           | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethene | N.D.  | 2.70   | 61.0 | 180.3     | 63.0 | 56.7      |



| Compound           | Conc.  | RT   | Dev(Min) | Resp.    | QIon | QRatio | Lower | Upper |
|--------------------|--------|------|----------|----------|------|--------|-------|-------|
| Methylene chloride | 1.2889 | 3.33 | -0.01    | 1664 (m) | 84.0 | 78.1   | 36.9  | 96.9  |
|                    |        |      |          |          | 86.0 | 31.4   | 14.3  | 74.3  |




# Quantitation Results Report (QT Reviewed)

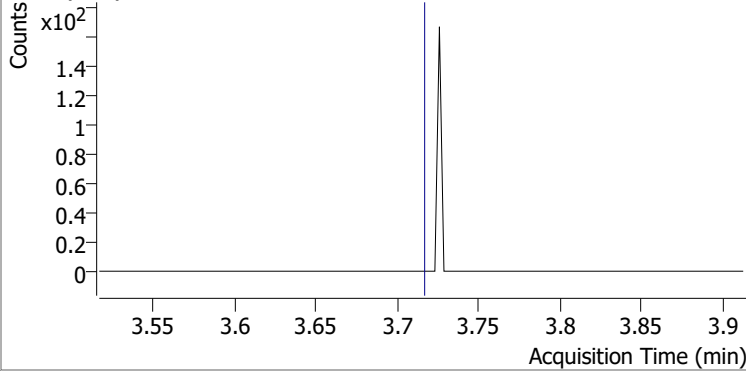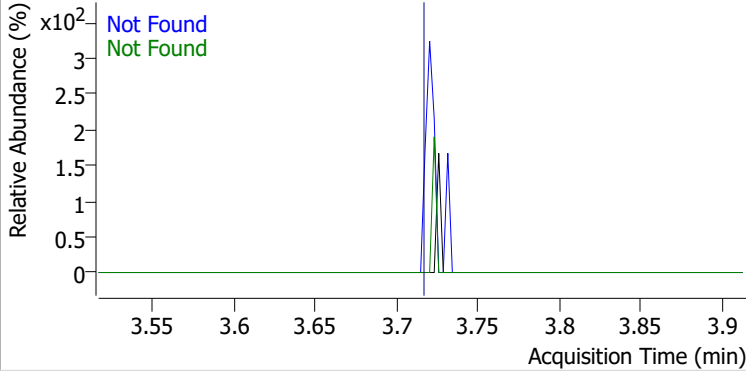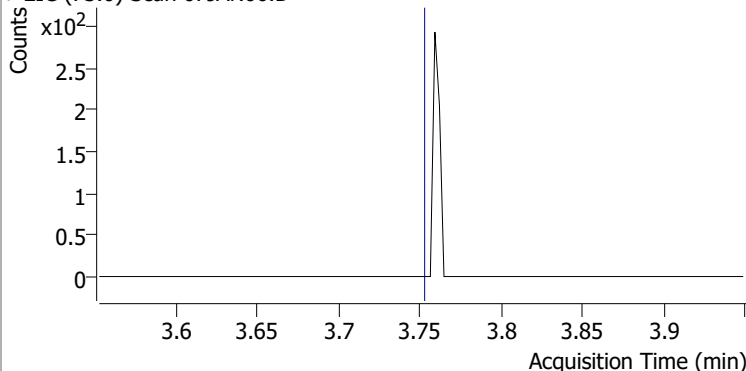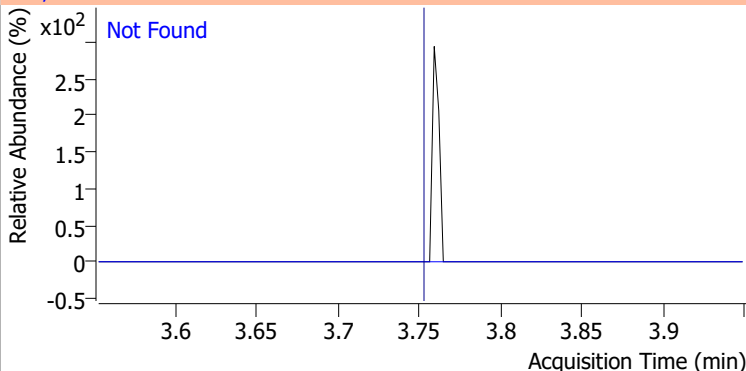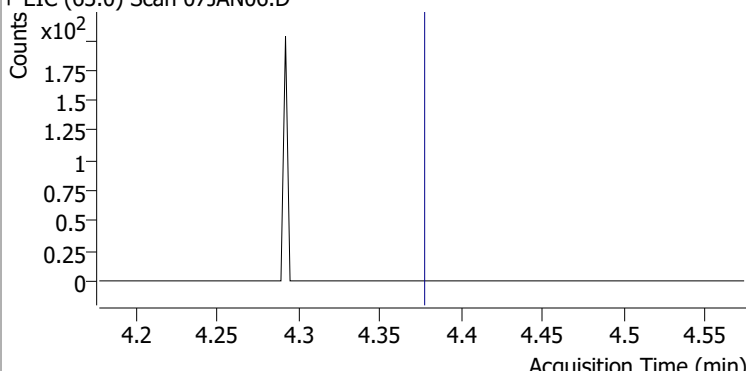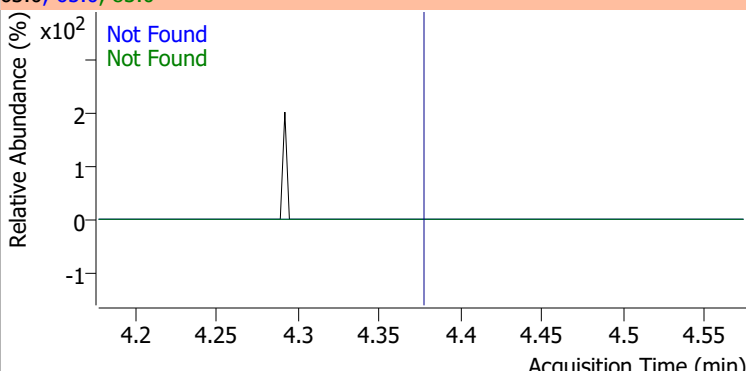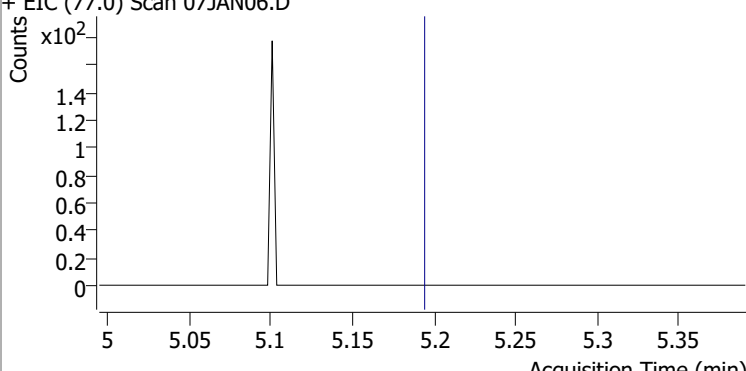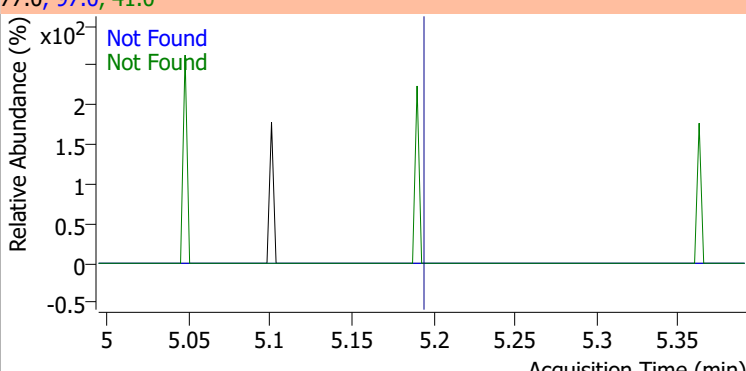
| Compound                                                                           | Conc. | Exp RT | QIon                                                                                 | Exp Ratio | QIon | Exp Ratio |
|------------------------------------------------------------------------------------|-------|--------|--------------------------------------------------------------------------------------|-----------|------|-----------|
| trans-1,2-Dichloroethene                                                           | N.D.  | 3.72   | 61.0                                                                                 | 153.9     | 98.0 | 65.7      |
| + EIC (96.0) Scan 07JAN06.D                                                        |       |        | 96.0, 61.0, 98.0                                                                     |           |      |           |
|    |       |        |    |           |      |           |
| Methyl tert-butyl ether (MTBE)                                                     | N.D.  | 3.75   | 57.0                                                                                 | 24.6      |      |           |
| + EIC (73.0) Scan 07JAN06.D                                                        |       |        | 73.0, 57.0                                                                           |           |      |           |
|   |       |        |   |           |      |           |
| 1,1-Dichloroethane                                                                 | N.D.  | 4.38   | 65.0                                                                                 | 32.1      | 83.0 | 13.7      |
| + EIC (63.0) Scan 07JAN06.D                                                        |       |        | 63.0, 65.0, 83.0                                                                     |           |      |           |
|  |       |        |  |           |      |           |
| 2,2-Dichloropropane                                                                | N.D.  | 5.20   | 41.0                                                                                 | 66.5      | 97.0 | 23.2      |
| + EIC (77.0) Scan 07JAN06.D                                                        |       |        | 77.0, 97.0, 41.0                                                                     |           |      |           |
|  |       |        |  |           |      |           |

# Quantitation Results Report (QT Reviewed)


| Compound               | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|------------------------|-------|--------|------|-----------|------|-----------|
| cis-1,2-Dichloroethene | N.D.  | 5.22   | 61.0 | 167.2     | 98.0 | 67.3      |

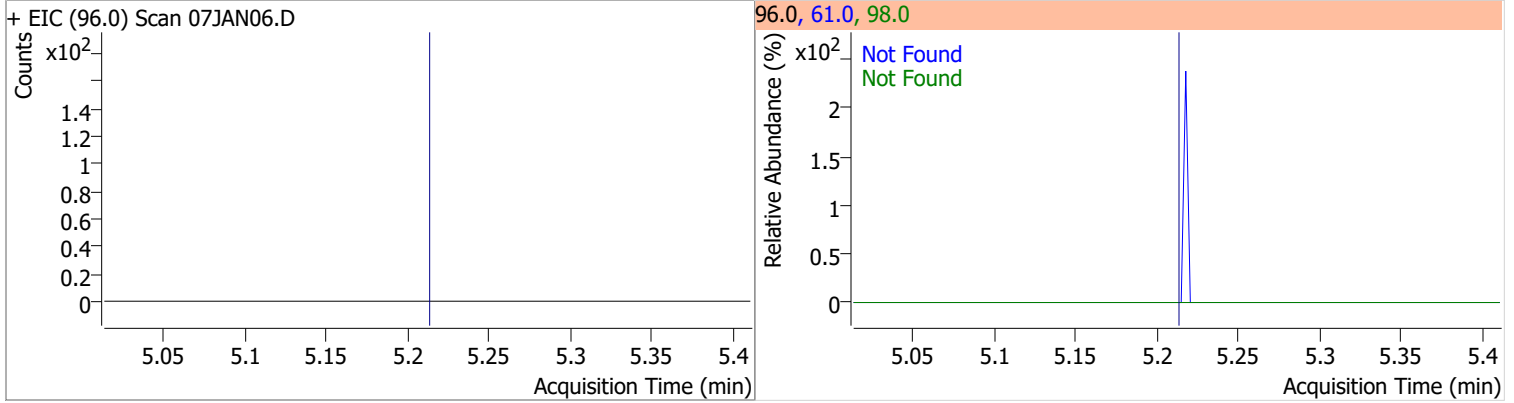


| Compound            | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| Methyl ethyl ketone | N.D.  | 5.28   | 72.0 | 21.3      |

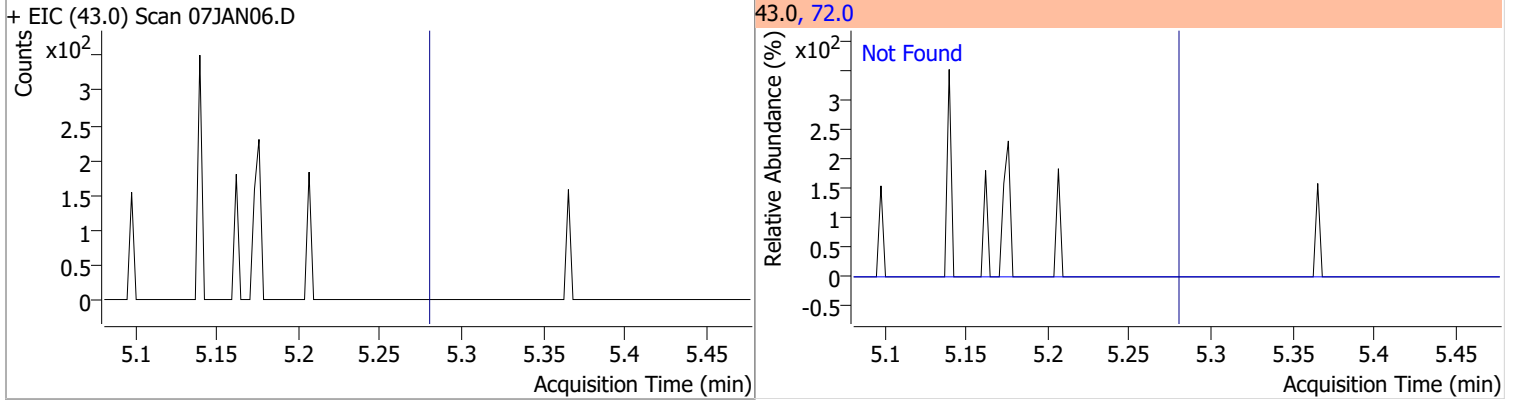





| Compound           | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|
| Bromochloromethane | N.D.  | 5.52   | 49.0 | 182.9     |

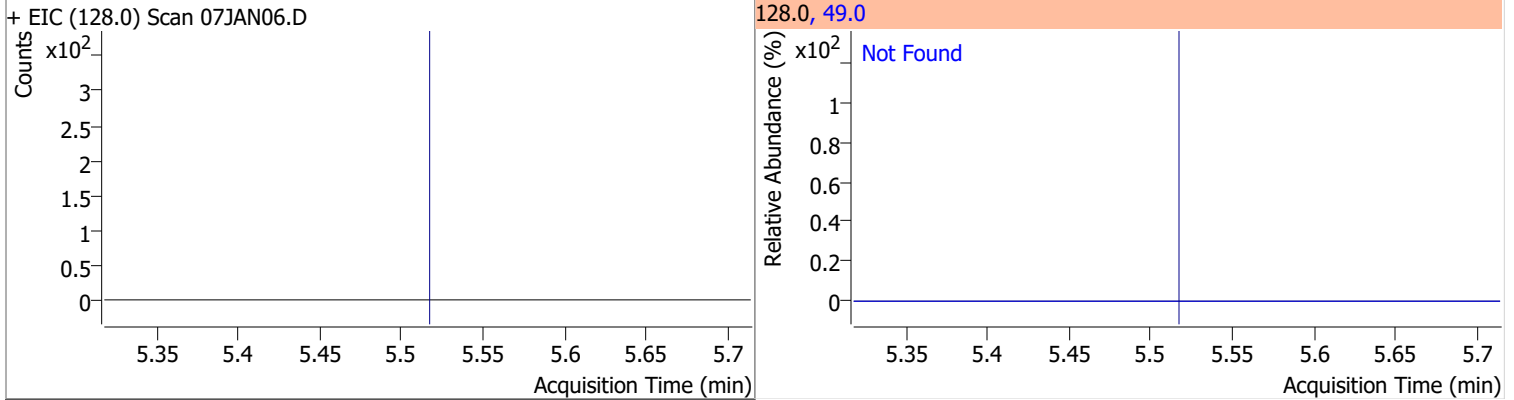

| Compound   | Conc. | Exp RT | QIon | Exp Ratio |
|------------|-------|--------|------|-----------|
| Chloroform | N.D.  | 5.65   | 85.0 | 66.0      |

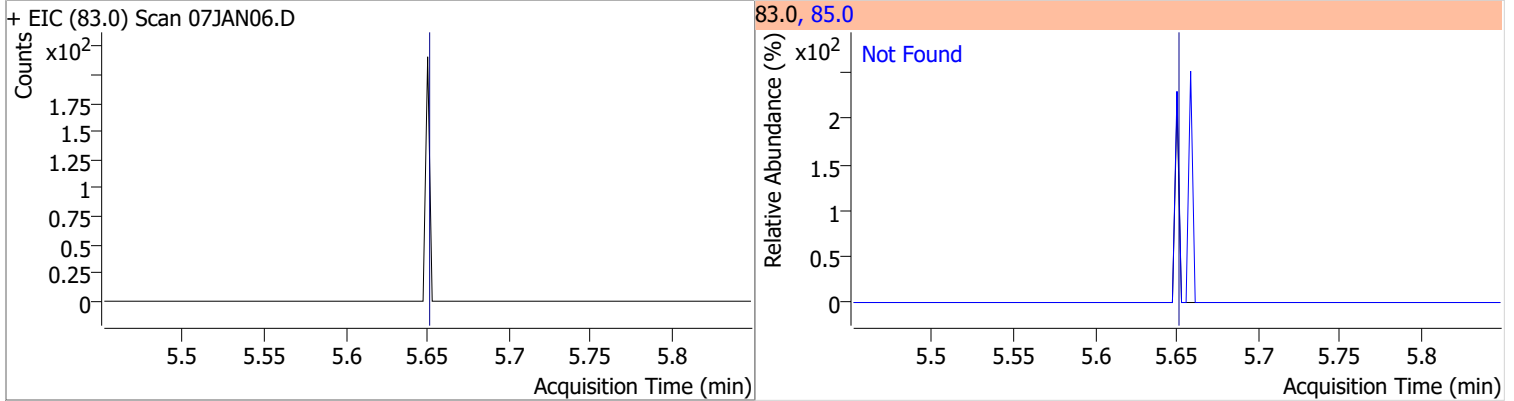


# Quantitation Results Report (QT Reviewed)

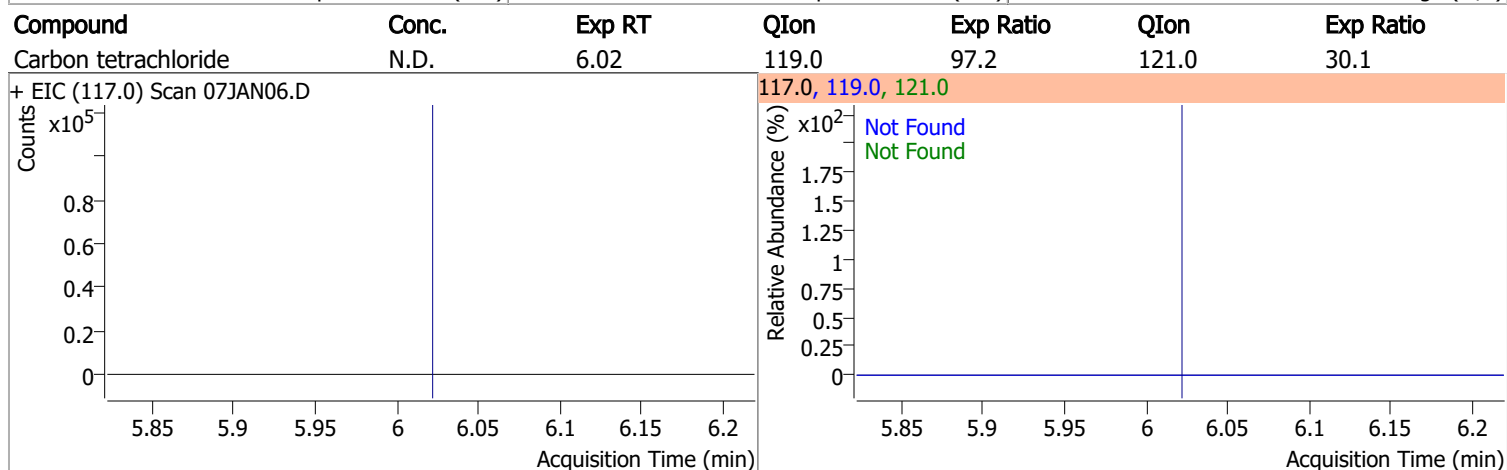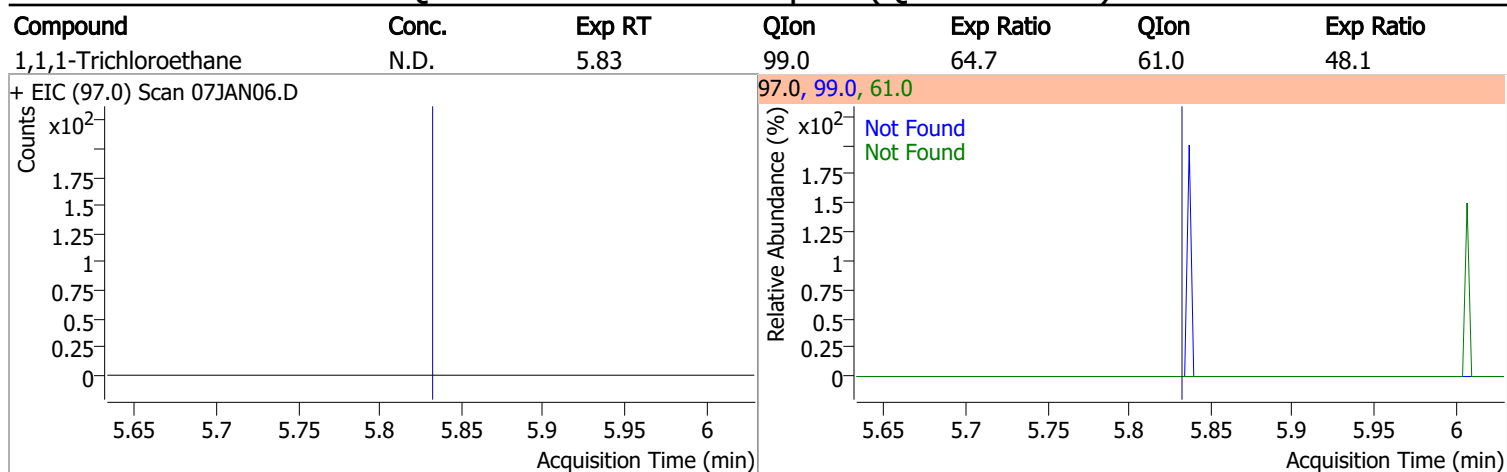


# Quantitation Results Report (QT Reviewed)


| Compound              | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 279.1458 | 6.23 | 0.00     | 98740 | 65.0 | 194.6  | 166.5 | 226.5 |

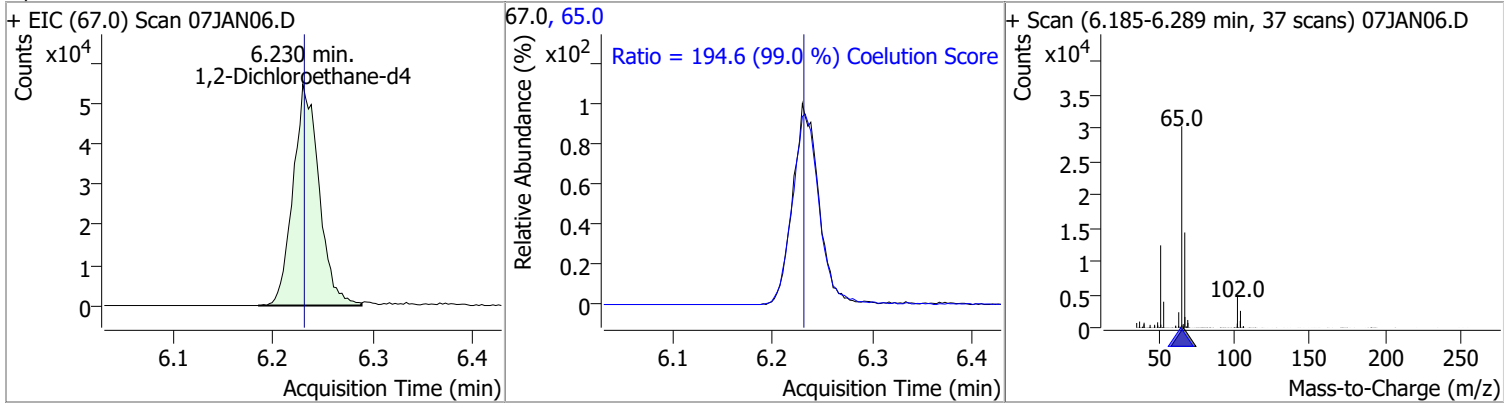


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------|-------|--------|------|-----------|
| Benzene  | N.D.  | 6.28   | 77.0 | 23.5      |

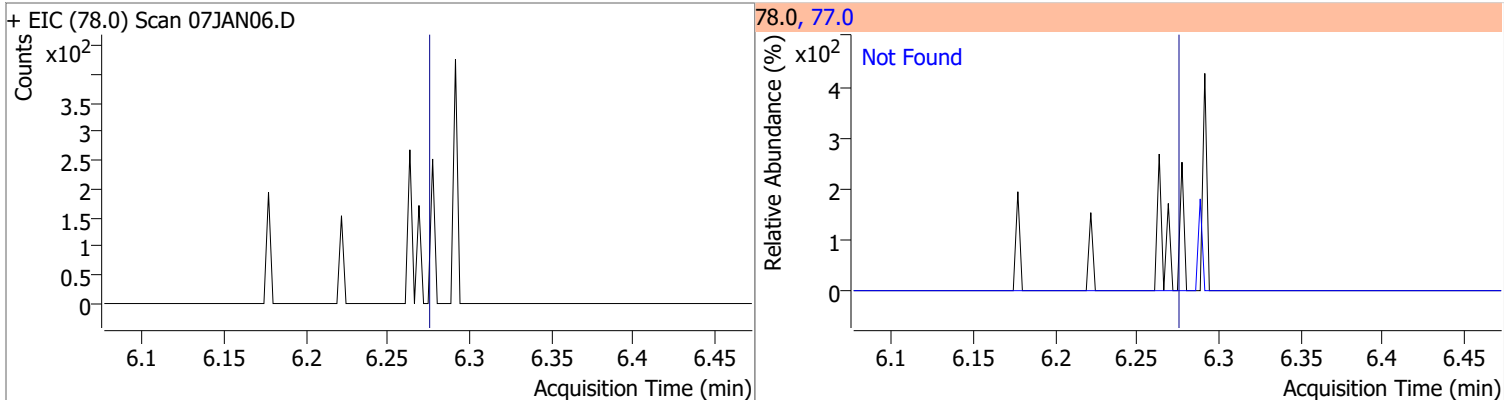

| Compound           | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,2-Dichloroethane | N.D.  | 6.32   | 64.0 | 29.9      | 98.0 | 7.6       |




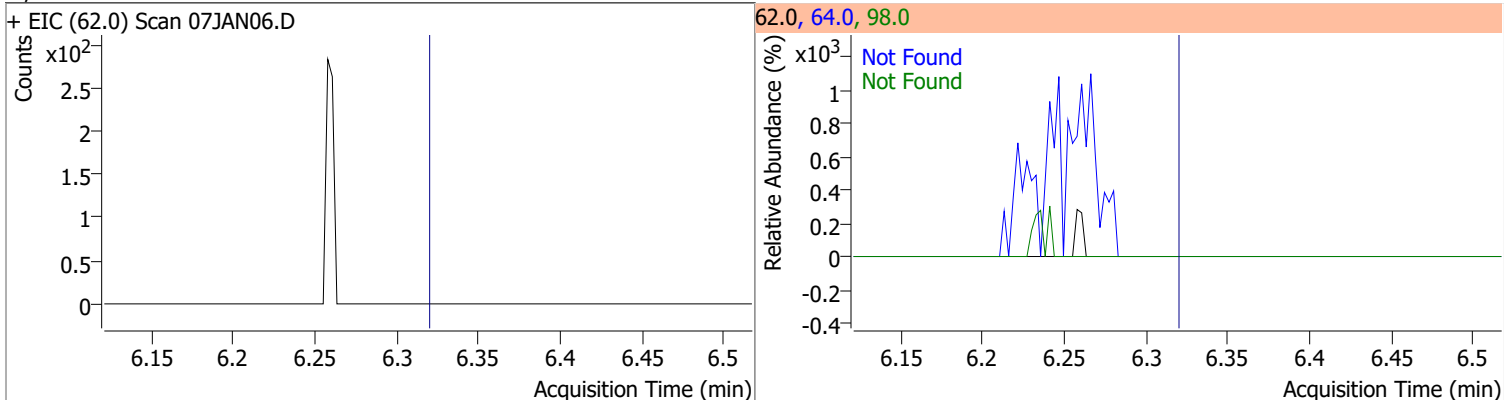


| Compound        | Conc. | Exp RT | QIon  | Exp Ratio | QIon | Exp Ratio |
|-----------------|-------|--------|-------|-----------|------|-----------|
| Trichloroethene | N.D.  | 7.03   | 130.0 | 101.5     | 97.0 | 64.1      |

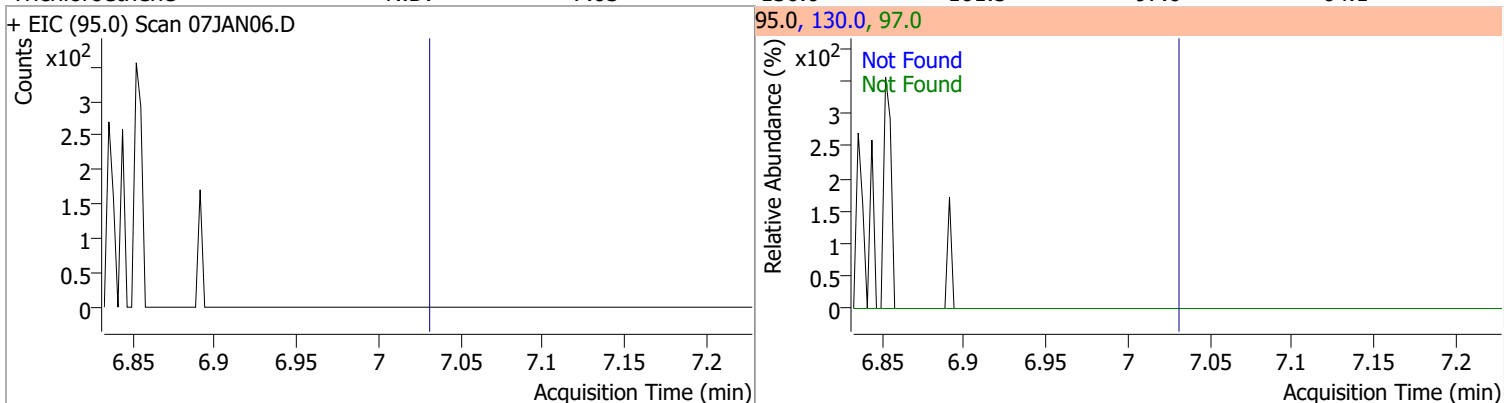




# Quantitation Results Report (QT Reviewed)

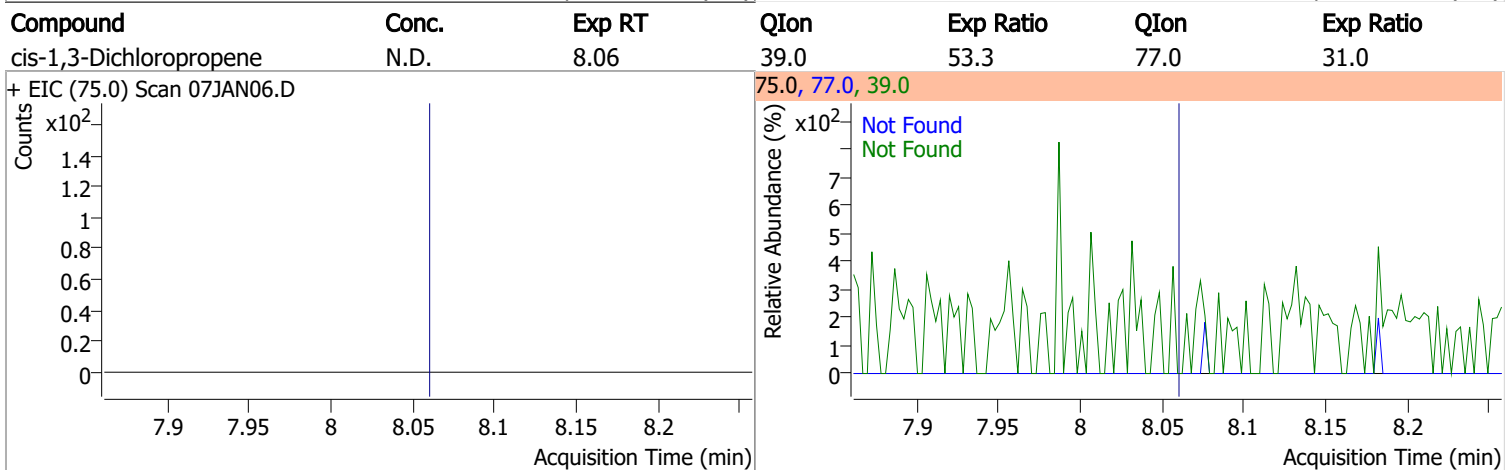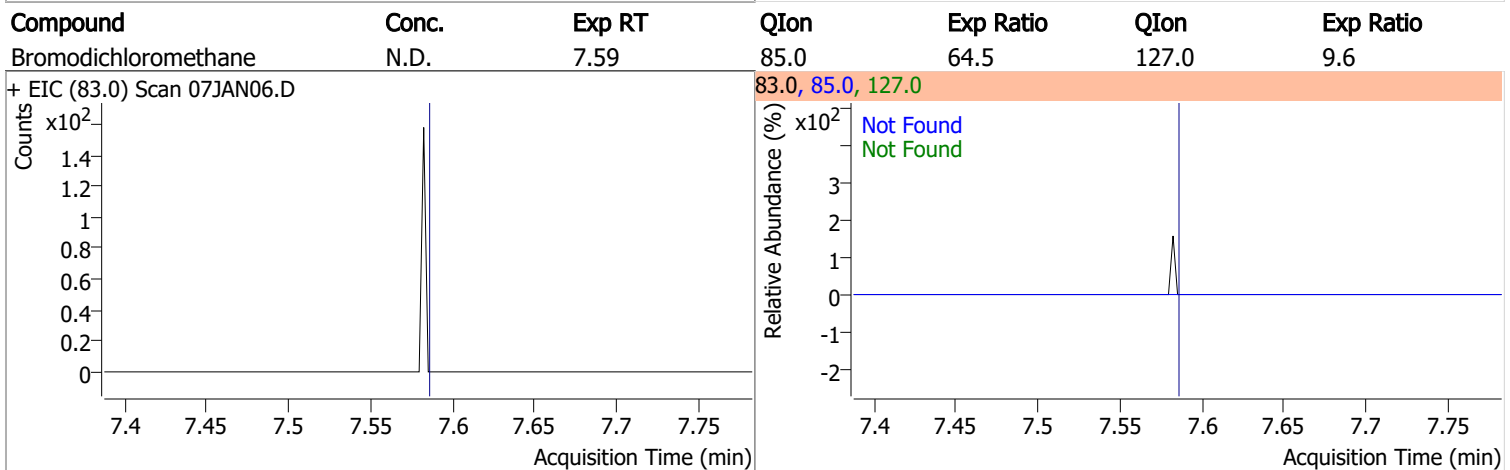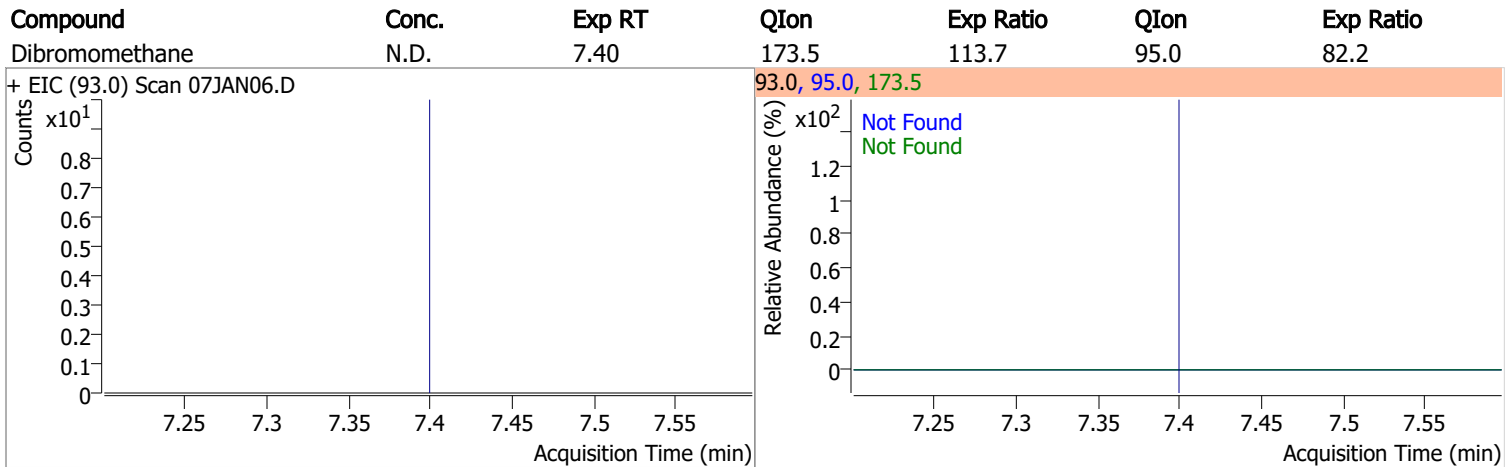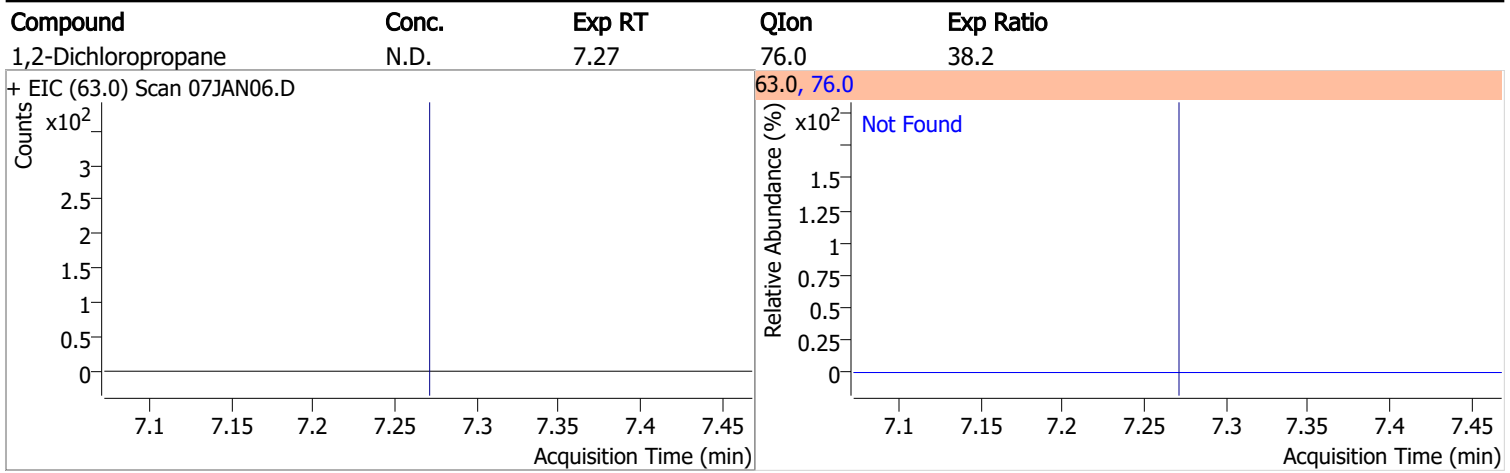


# Quantitation Results Report (QT Reviewed)


| Compound   | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 264.3775 | 8.32 | 0.00     | 864903 | 100.0 | 63.8   | 34.4  | 94.4  |
|            |          |      |          |        | 99.0  | 9.5    | 0.0   | 39.6  |

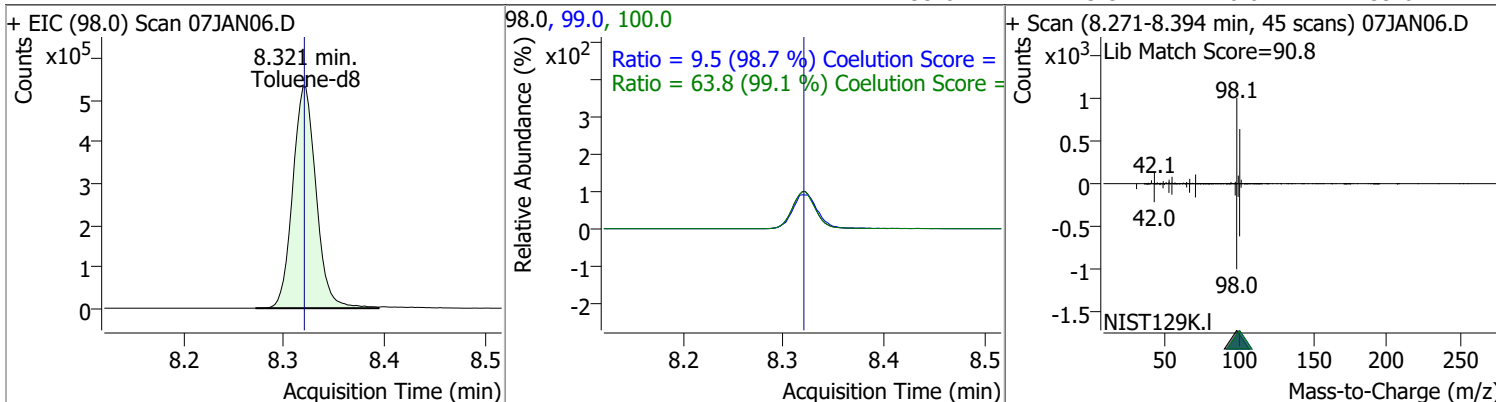


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------|-------|--------|------|-----------|
| Toluene  | N.D.  | 8.39   | 91.0 | 175.8     |

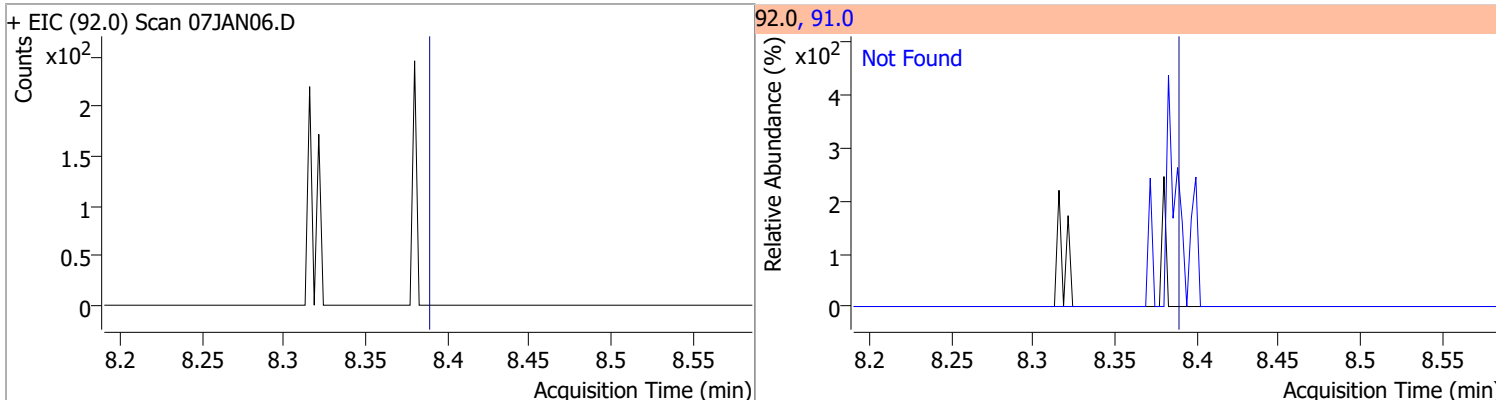





| Compound                  | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,3-Dichloropropene | N.D.  | 8.64   | 39.0 | 53.4      | 77.0 | 32.4      |

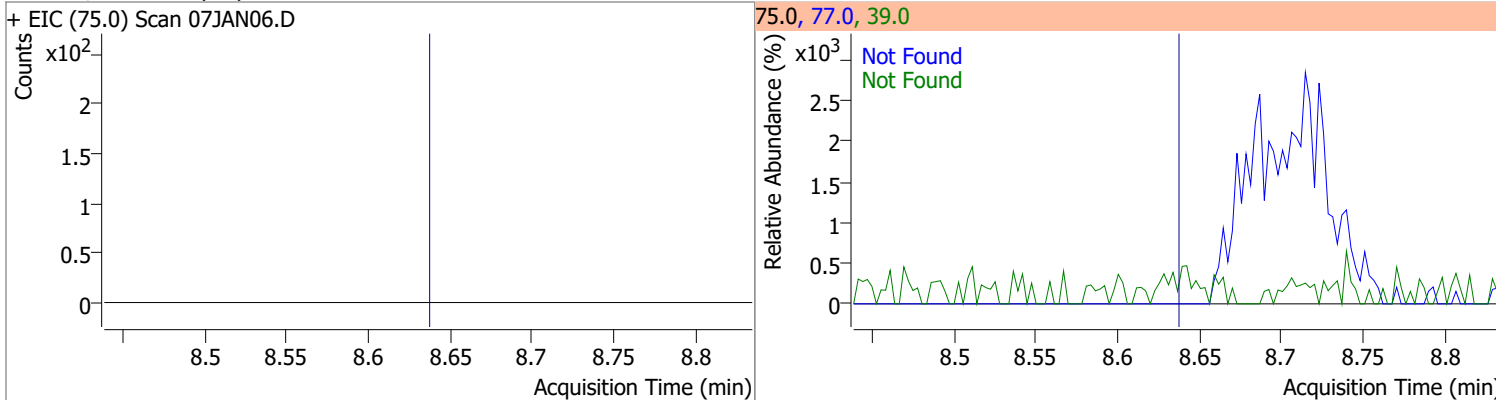









| Compound              | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------------|-------|--------|------|-----------|------|-----------|
| 1,1,2-Trichloroethane | N.D.  | 8.82   | 97.0 | 114.6     | 85.0 | 67.6      |

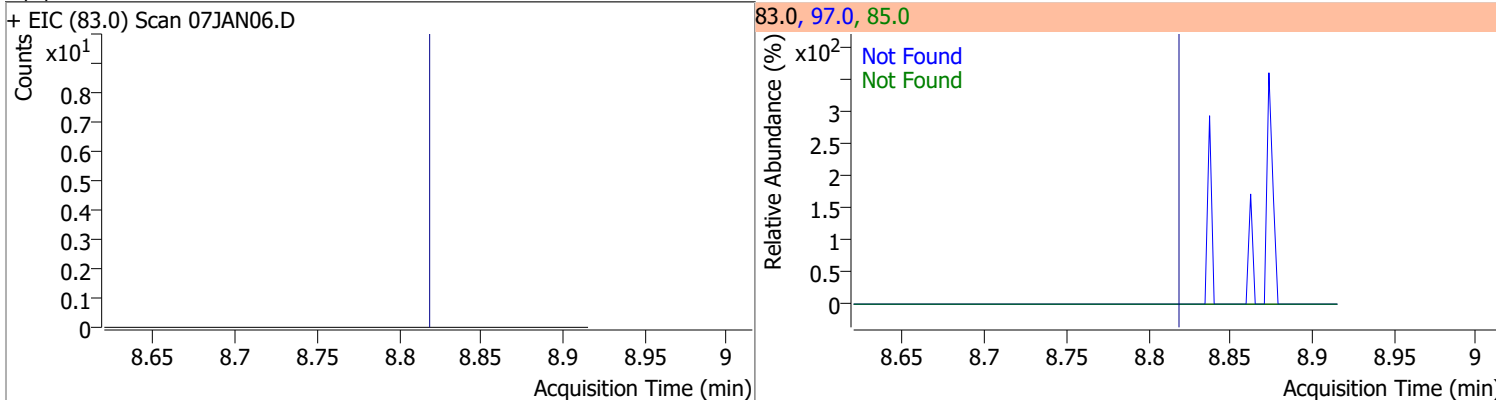




# Quantitation Results Report (QT Reviewed)




# Quantitation Results Report (QT Reviewed)
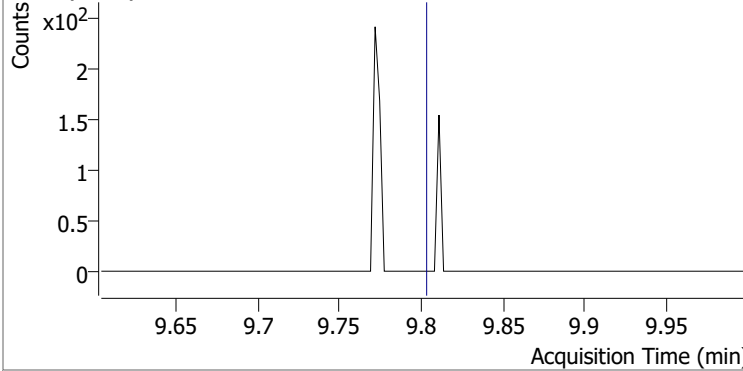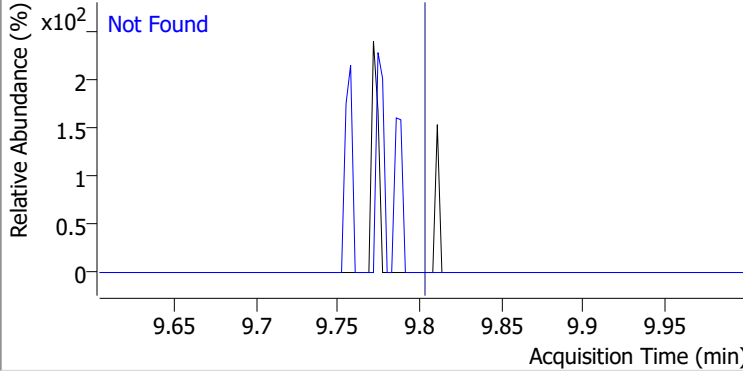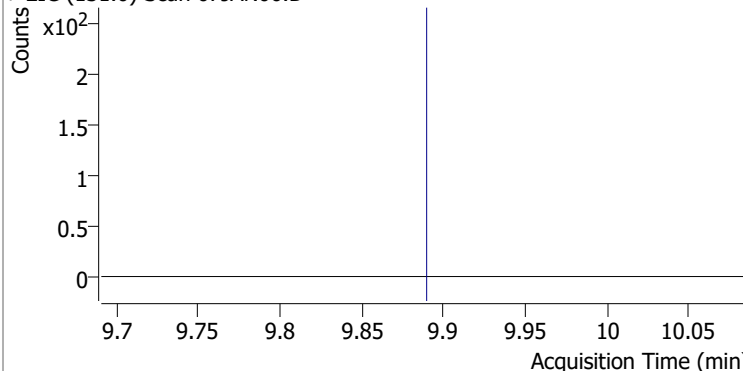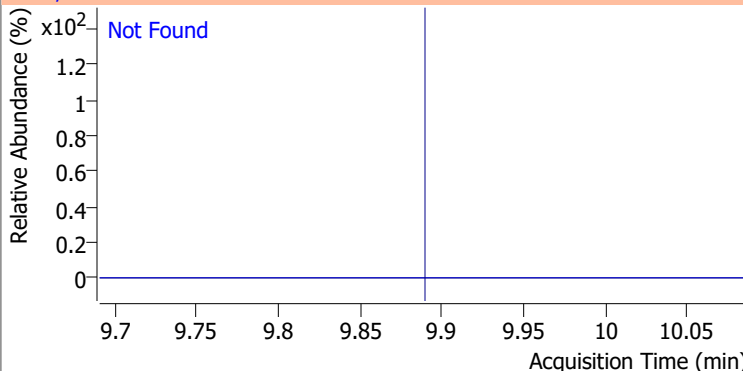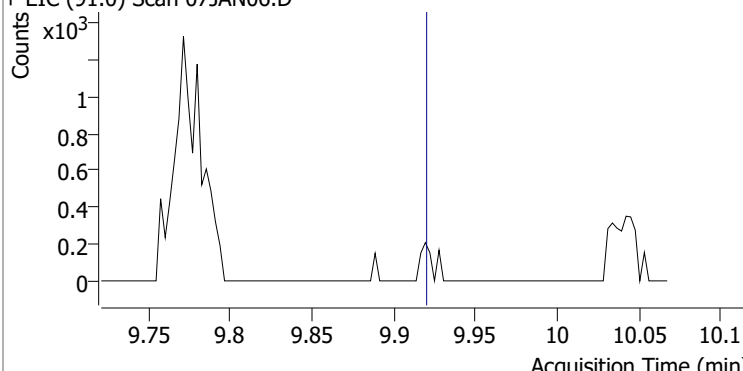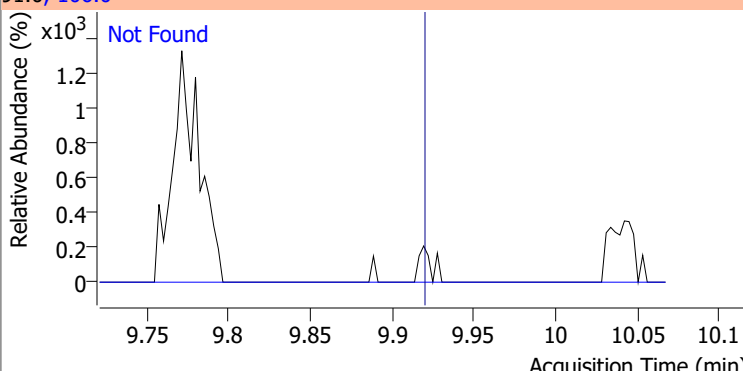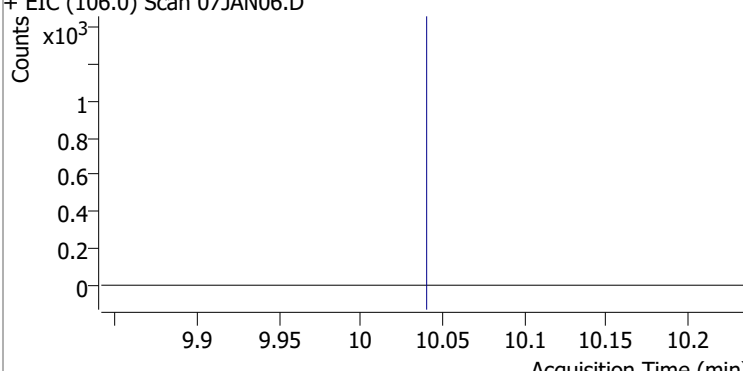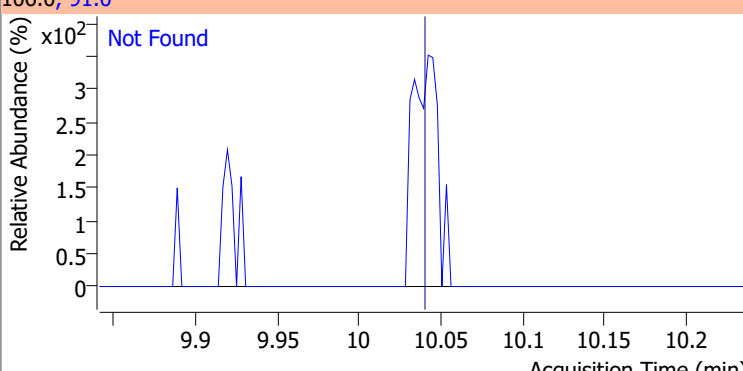
| Compound                                                                           | Conc. | Exp RT | QIon                                                                                 | Exp Ratio |
|------------------------------------------------------------------------------------|-------|--------|--------------------------------------------------------------------------------------|-----------|
| Chlorobenzene                                                                      | N.D.  | 9.80   | 114.0                                                                                | 32.1      |
| + EIC (112.0) Scan 07JAN06.D                                                       |       |        | 112.0, 114.0                                                                         |           |
|    |       |        |    |           |
| 1,1,1,2-Tetrachloroethane                                                          | N.D.  | 9.89   | 133.0                                                                                | 98.6      |
| + EIC (131.0) Scan 07JAN06.D                                                       |       |        | 131.0, 133.0                                                                         |           |
|   |       |        |   |           |
| Ethylbenzene                                                                       | N.D.  | 9.92   | 106.0                                                                                | 31.1      |
| + EIC (91.0) Scan 07JAN06.D                                                        |       |        | 91.0, 106.0                                                                          |           |
|  |       |        |  |           |
| m+p-Xylenes                                                                        | N.D.  | 10.04  | 91.0                                                                                 | 201.4     |
| + EIC (106.0) Scan 07JAN06.D                                                       |       |        | 106.0, 91.0                                                                          |           |
|  |       |        |  |           |









# Quantitation Results Report (QT Reviewed)

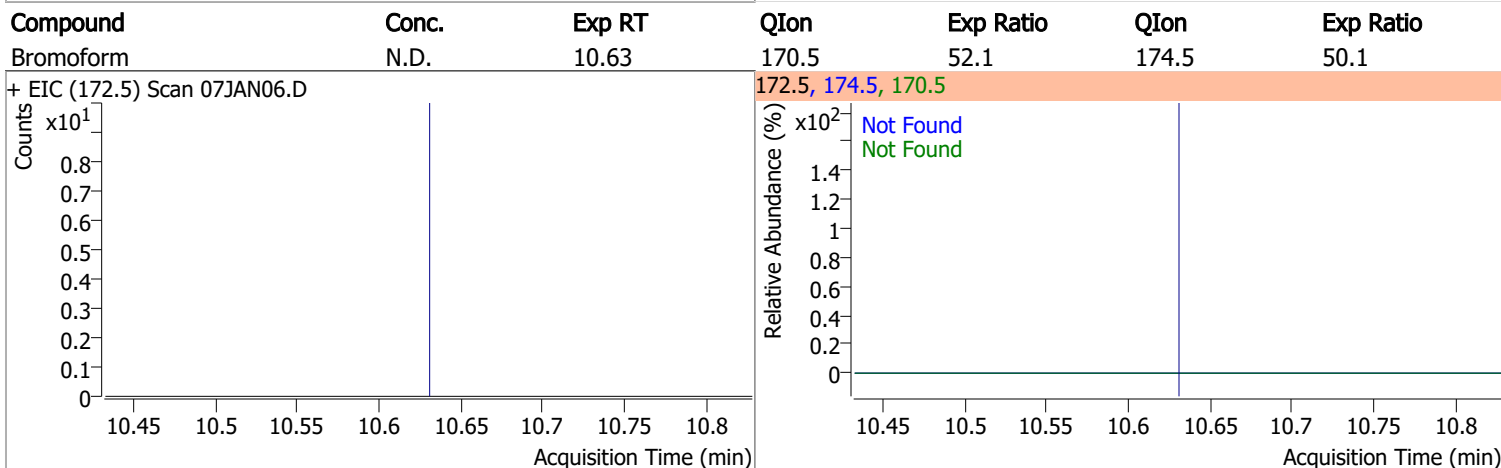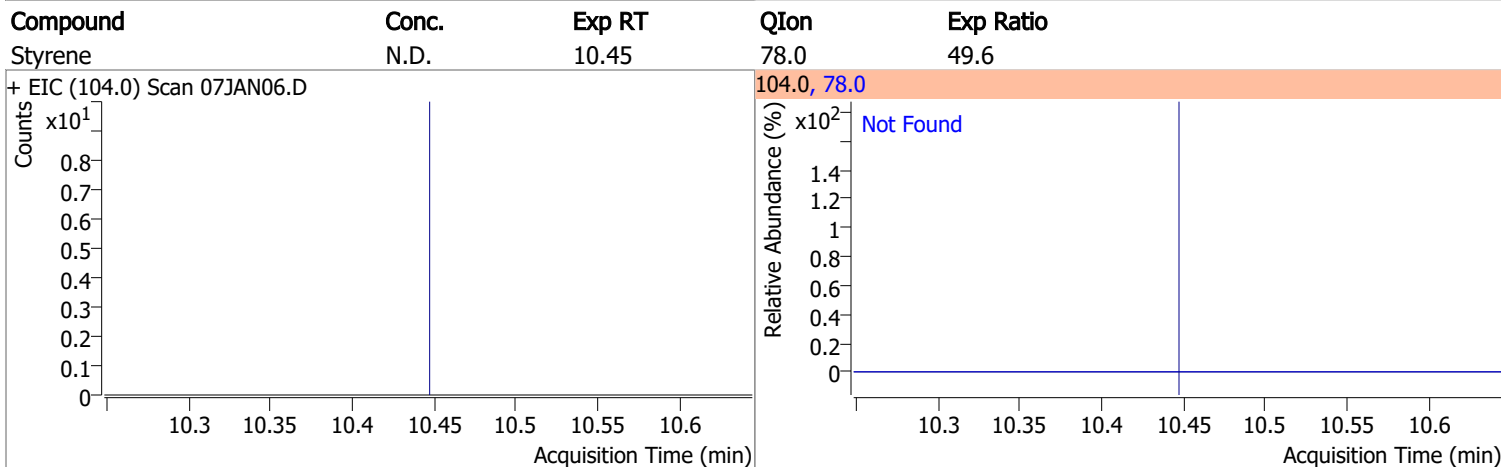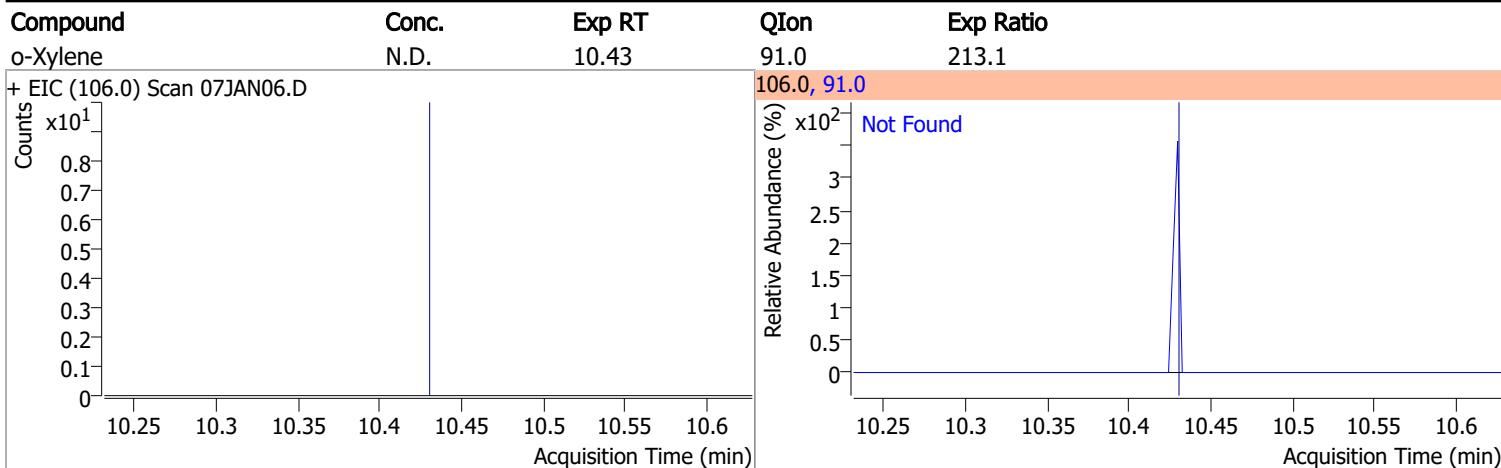









| Compound             | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 274.9894 | 10.95 | 0.00     | 259344 | 174.0 | 91.2   | 61.7  | 121.7 |
|                      |          |       |          |        | 176.0 | 89.1   | 60.6  | 120.6 |

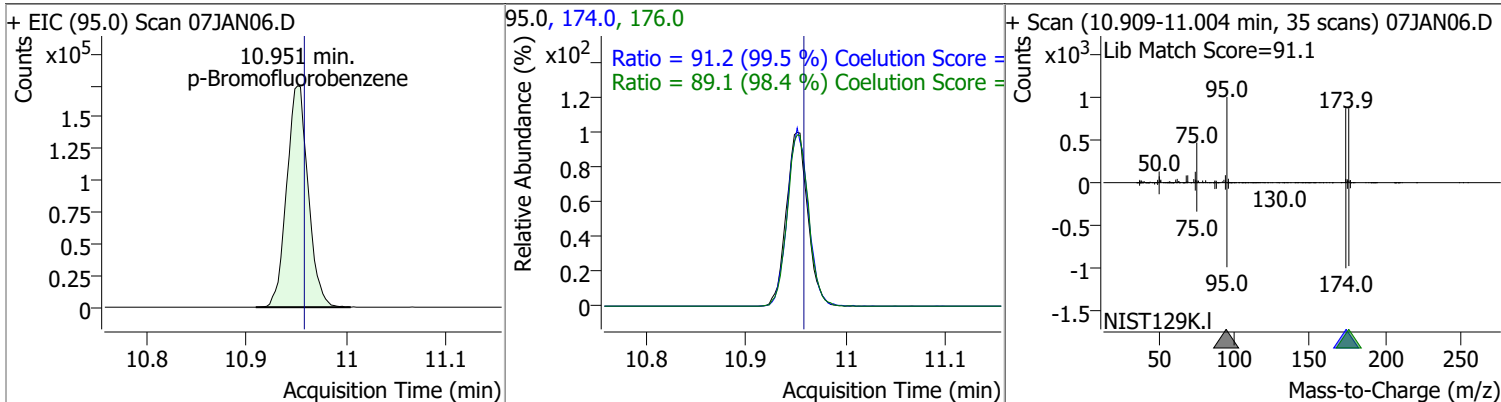

# Quantitation Results Report (QT Reviewed)

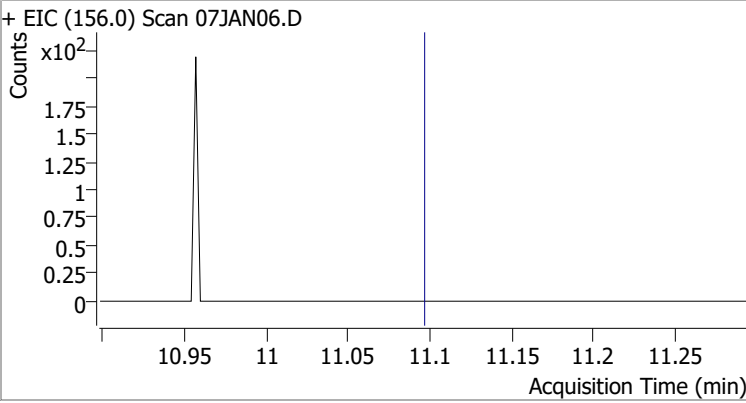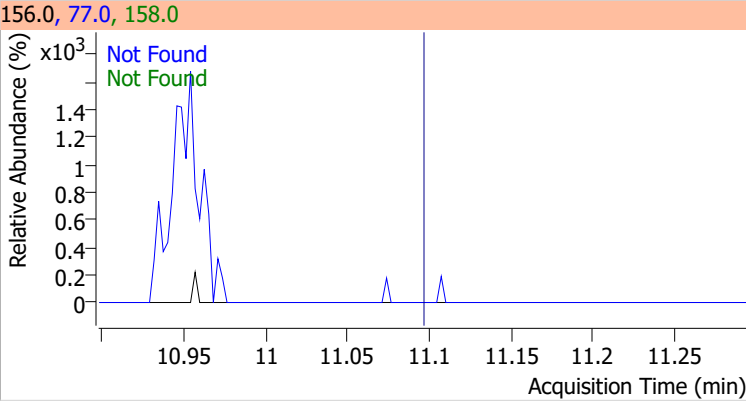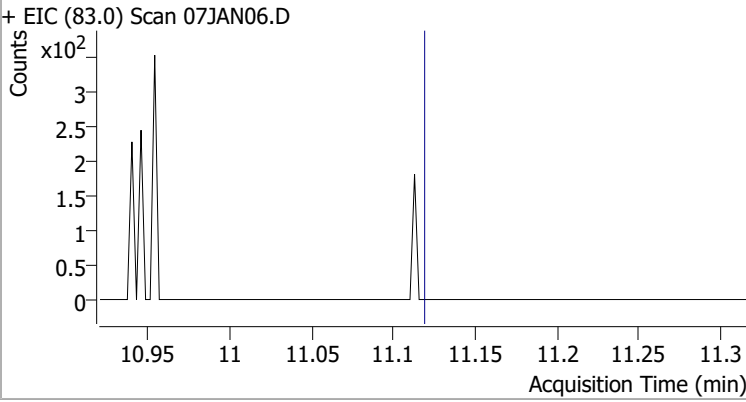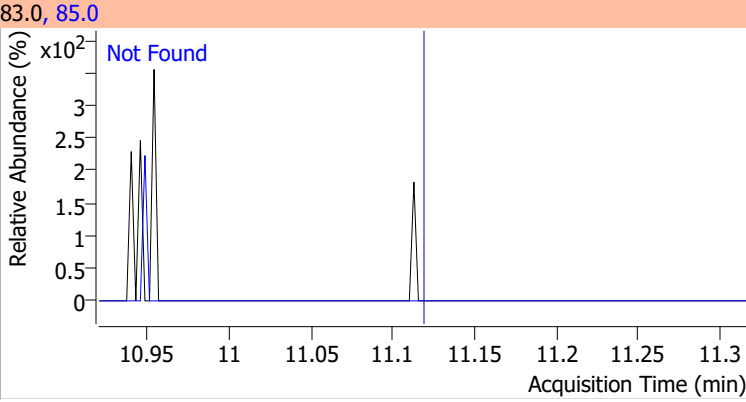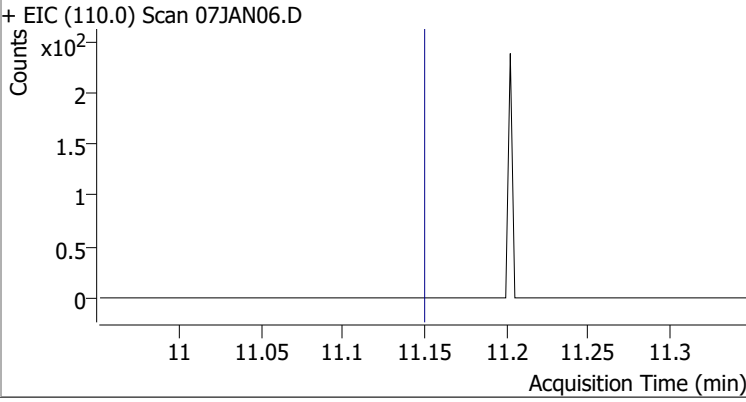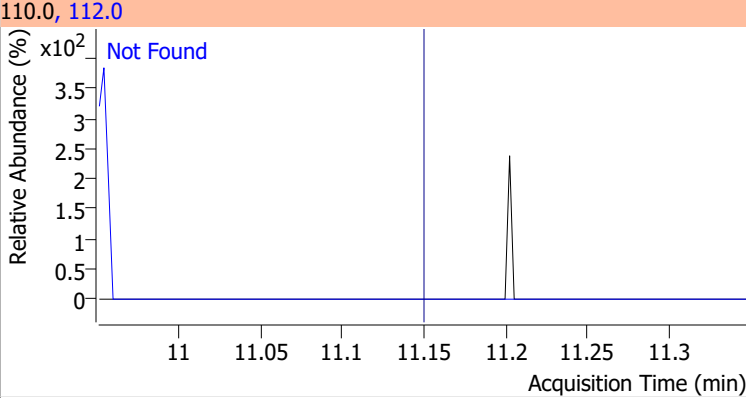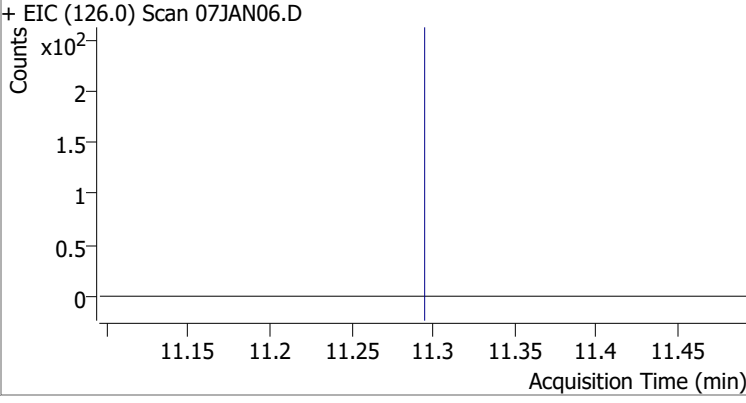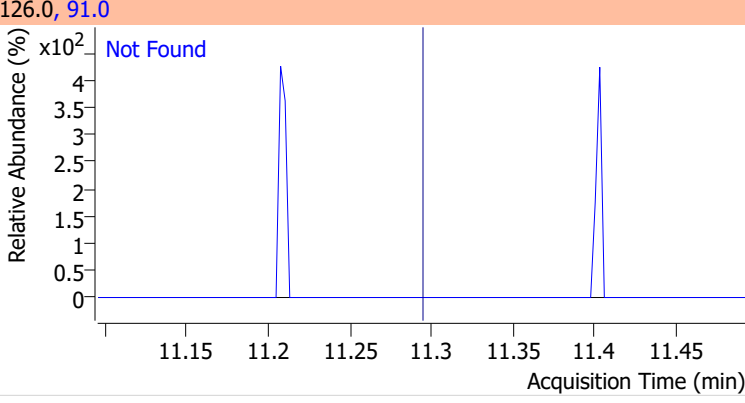
| Compound                                                                           | Conc. | Exp RT | QIon                                                                                 | Exp Ratio | QIon  | Exp Ratio |
|------------------------------------------------------------------------------------|-------|--------|--------------------------------------------------------------------------------------|-----------|-------|-----------|
| Bromobenzene                                                                       | N.D.  | 11.09  | 77.0                                                                                 | 145.7     | 158.0 | 96.5      |
| + EIC (156.0) Scan 07JAN06.D                                                       |       |        | 156.0, 77.0, 158.0                                                                   |           |       |           |
|    |       |        |    |           |       |           |
| 1,1,2,2-Tetrachloroethane                                                          | N.D.  | 11.12  | 85.0                                                                                 | 66.2      |       |           |
| + EIC (83.0) Scan 07JAN06.D                                                        |       |        | 83.0, 85.0                                                                           |           |       |           |
|   |       |        |   |           |       |           |
| 1,2,3-Trichloropropane                                                             | N.D.  | 11.15  | 112.0                                                                                | 63.5      |       |           |
| + EIC (110.0) Scan 07JAN06.D                                                       |       |        | 110.0, 112.0                                                                         |           |       |           |
|  |       |        |  |           |       |           |
| 2-Chlorotoluene                                                                    | N.D.  | 11.29  | 91.0                                                                                 | 282.3     |       |           |
| + EIC (126.0) Scan 07JAN06.D                                                       |       |        | 126.0, 91.0                                                                          |           |       |           |
|  |       |        |  |           |       |           |

# Quantitation Results Report (QT Reviewed)
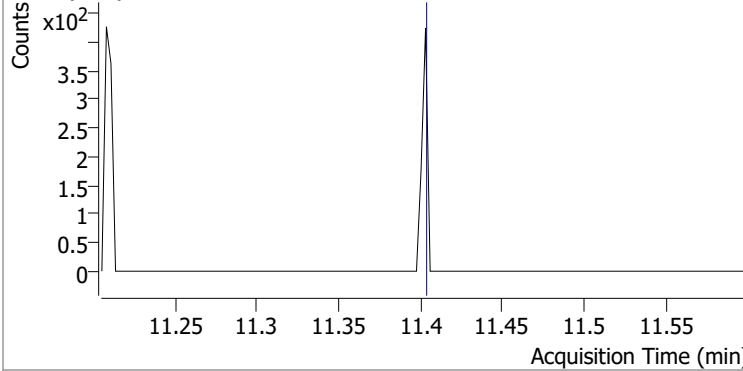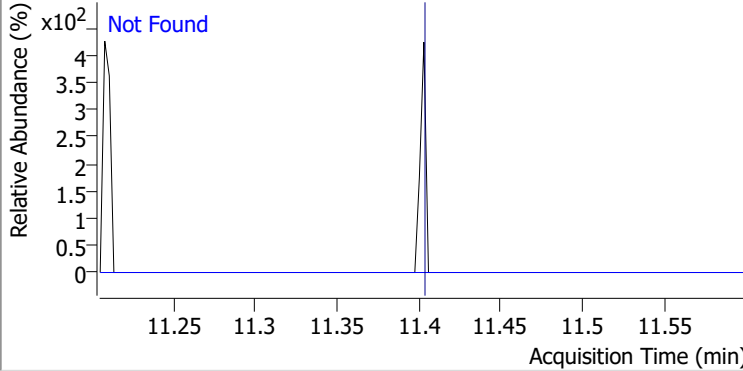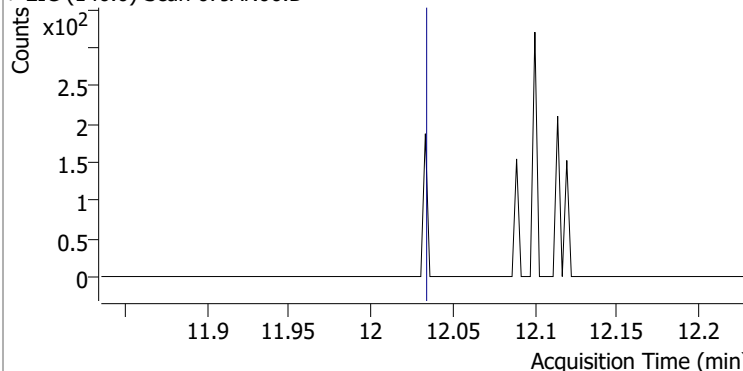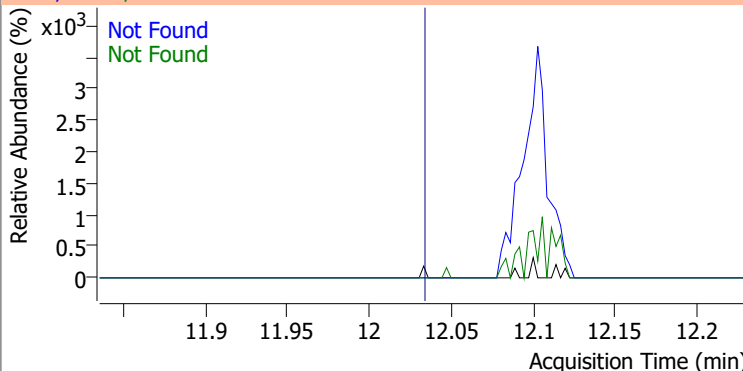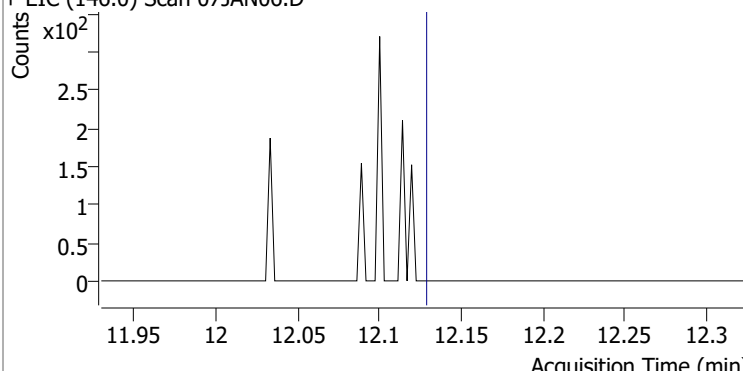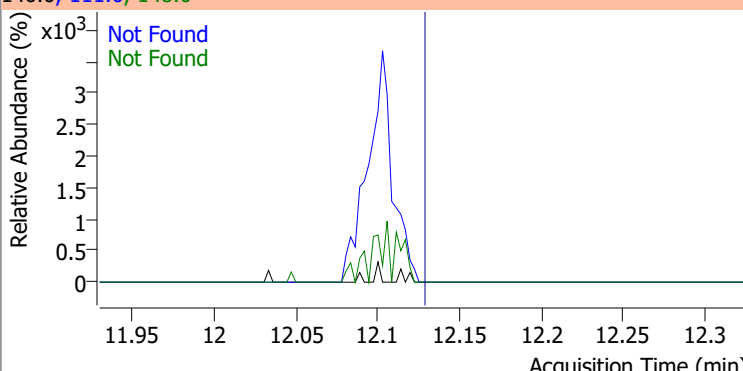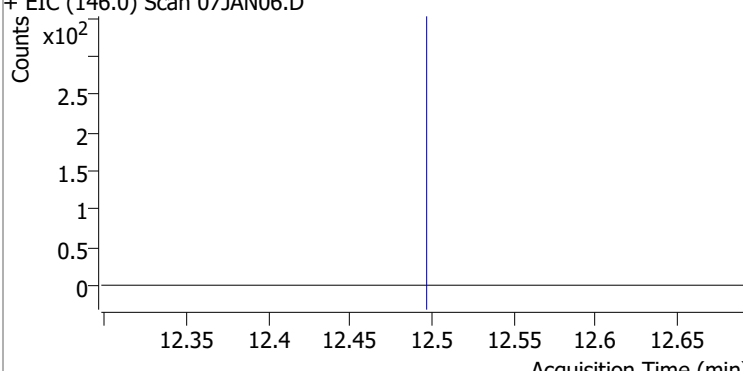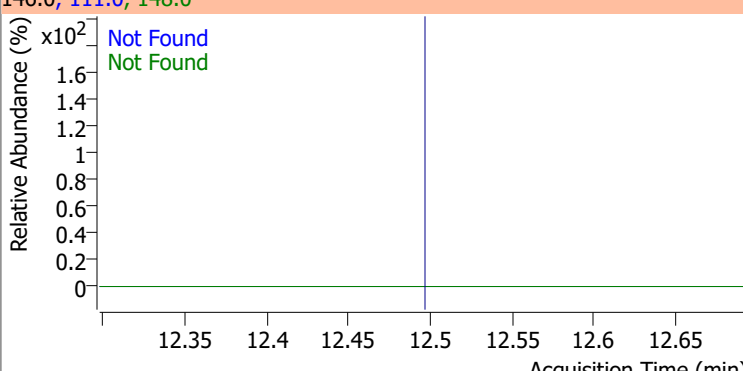
| Compound                                                                           | Conc. | Exp RT | QIon                                                                                 | Exp Ratio |      |           |
|------------------------------------------------------------------------------------|-------|--------|--------------------------------------------------------------------------------------|-----------|------|-----------|
| 4-Chlorotoluene                                                                    | N.D.  | 11.40  | 126.0                                                                                | 31.7      |      |           |
| + EIC (91.0) Scan 07JAN06.D                                                        |       |        | 91.0, 126.0                                                                          |           |      |           |
|    |       |        |    |           |      |           |
| 1,3-Dichlorobenzene                                                                | N.D.  | 12.03  | 148.0                                                                                | 63.6      | QIon | Exp Ratio |
| + EIC (146.0) Scan 07JAN06.D                                                       |       |        | 146.0, 111.0, 148.0                                                                  |           |      |           |
|   |       |        |   |           |      |           |
| 1,4-Dichlorobenzene                                                                | N.D.  | 12.13  | 148.0                                                                                | 63.1      | QIon | Exp Ratio |
| + EIC (146.0) Scan 07JAN06.D                                                       |       |        | 146.0, 111.0, 148.0                                                                  |           |      |           |
|  |       |        |  |           |      |           |
| 1,2-Dichlorobenzene                                                                | N.D.  | 12.49  | 148.0                                                                                | 63.9      | QIon | Exp Ratio |
| + EIC (146.0) Scan 07JAN06.D                                                       |       |        | 146.0, 111.0, 148.0                                                                  |           |      |           |
|  |       |        |  |           |      |           |

# Quantitation Results Report (QT Reviewed)

|                |                                     |                   |                       |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File      | 07JAN07.D                           | Operator          | MSC                   |
| Acq. Method    | 5975CACQF.M                         | Acq. Date-Time    | 1/7/2022 12:24:50 PM  |
| Sample Name    | B22010214-002A                      | Instrument        | VOA5975C              |
| Vial           | 7                                   | Multiplier        | 1.00                  |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m  | Comment           |                       |
| Tune File      | BFB_Atune3.u                        | Tune Date         | 10/11/2021 4:02:00 PM |
| Batch Name     | VG010722_8260B.batch.bin            | Last Calib Update | 3/2/2022 10:41:44 AM  |
| Ref Library    | \\MASSHUNTER\Org\Library\NIST129K.I |                   |                       |

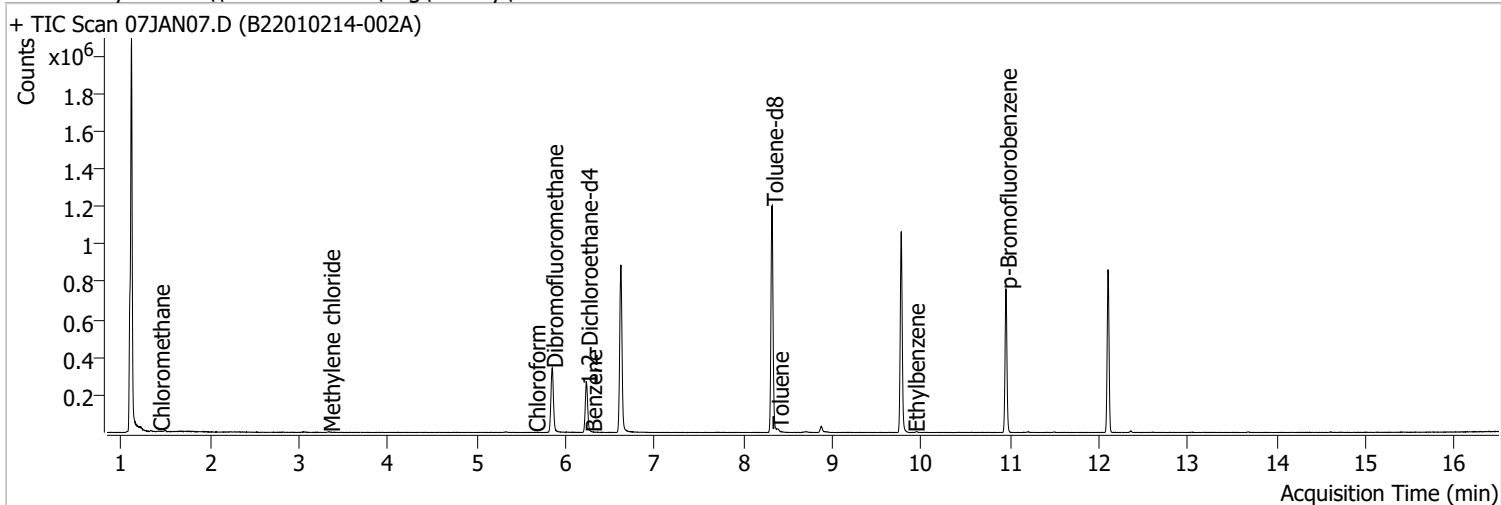

| Compound                           | RT                   | QIon  | Resp.  | Conc.                | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|----------------------|-------|----------|
| <b>Internal Standards</b>          |                      |       |        |                      |       |          |
| M Fluorobenzene                    | 6.620                | 96.0  | 753037 | 250.0000             | ng    | -0.003   |
| M Chlorobenzene-d5                 | 9.774                | 82.0  | 295673 | 250.0000             | ng    | 0.003    |
| M 1,4-Dichlorobenzene-d4           | 12.100               | 152.0 | 207588 | 250.0000             | ng    | 0.000    |
| <b>System Monitoring Compounds</b> |                      |       |        |                      |       |          |
| S Dibromofluoromethane             | 5.848                | 113.0 | 207577 | 292.5939             | ng    | 0.003    |
| Spiked Amount: 250.000             | Range: 80.0 - 119.0% |       |        | Recovery = 117.04%   |       |          |
| S 1,2-Dichloroethane-d4            | 6.236                | 67.0  | 96449  | 314.7549             | ng    | 0.003    |
| Spiked Amount: 250.000             | Range: 81.0 - 118.0% |       |        | Recovery = 125.90% * |       |          |
| S Toluene-d8                       | 8.321                | 98.0  | 740894 | 260.0307             | ng    | 0.003    |
| Spiked Amount: 250.000             | Range: 89.0 - 112.0% |       |        | Recovery = 104.01%   |       |          |
| S p-Bromofluorobenzene             | 10.951               | 95.0  | 215644 | 283.5551             | ng    | -0.003   |
| Spiked Amount: 250.000             | Range: 85.0 - 114.0% |       |        | Recovery = 113.42%   |       |          |
| <b>Target Compounds</b>            |                      |       |        |                      |       |          |
| T Dichlorodifluoromethane          | 0.000                |       | 0      | N.D.                 |       |          |
| T Chloromethane                    | 1.422                | 50.0  | 1730   | 1.4445               | ng m  | 98       |
| T Vinyl chloride                   | 0.000                |       | 0      | N.D.                 |       |          |
| T Bromomethane                     | 0.000                |       | 0      | N.D.                 |       |          |
| T Chloroethane                     | 0.000                |       | 0      | N.D.                 |       |          |
| T Trichlorofluoromethane           | 0.000                |       | 0      | N.D.                 |       |          |
| T 1,1-Dichloroethene               | 0.000                |       | 0      | N.D.                 |       |          |
| T Methylene chloride               | 3.338                | 49.0  | 2222   | 1.9869               | ng m  | 91       |
| T trans-1,2-Dichloroethene         | 0.000                |       | 0      | N.D.                 |       |          |
| T Methyl tert-butyl ether (MTBE)   | 0.000                |       | 0      | N.D.                 |       |          |
| T 1,1-Dichloroethane               | 0.000                |       | 0      | N.D.                 |       |          |
| T 2,2-Dichloropropane              | 0.000                |       | 0      | N.D.                 |       |          |
| T cis-1,2-Dichloroethene           | 0.000                |       | 0      | N.D.                 |       |          |
| T Methyl ethyl ketone              | 0.000                |       | 0      | N.D.                 |       |          |
| T Bromochloromethane               | 0.000                |       | 0      | N.D.                 |       |          |
| T Chloroform                       | 5.647                | 83.0  | 209    | 0.1455               | ng m  | 80       |




# Quantitation Results Report (QT Reviewed)

| Compound                    | RT     | QIon  | Resp. | Conc.  | Units |    | Dev(Min) |
|-----------------------------|--------|-------|-------|--------|-------|----|----------|
| T 1,1,1-Trichloroethane     | 0.000  |       | 0     | N.D.   |       |    |          |
| T Carbon tetrachloride      | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,1-Dichloropropene       | 0.000  |       | 0     | N.D.   |       |    |          |
| T Benzene                   | 6.286  | 78.0  | 144   | 0.0480 | ng    | m  | 89       |
| T 1,2-Dichloroethane        | 0.000  |       | 0     | N.D.   |       |    |          |
| T Trichloroethene           | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,2-Dichloropropane       | 0.000  |       | 0     | N.D.   |       |    |          |
| T Dibromomethane            | 0.000  |       | 0     | N.D.   |       |    |          |
| T Bromodichloromethane      | 0.000  |       | 0     | N.D.   |       |    |          |
| T cis-1,3-Dichloropropene   | 0.000  |       | 0     | N.D.   |       |    |          |
| T Toluene                   | 8.386  | 92.0  | 3845  | 1.9977 | ng    |    | 100      |
| T trans-1,3-Dichloropropene | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,1,2-Trichloroethane     | 0.000  |       | 0     | N.D.   |       |    |          |
| T Tetrachloroethene         | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,3-Dichloropropane       | 0.000  |       | 0     | N.D.   |       |    |          |
| T Chlorodibromomethane      | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,2-Dibromoethane         | 0.000  |       | 0     | N.D.   |       |    |          |
| T Chlorobenzene             | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,1,1,2-Tetrachloroethane | 0.000  |       | 0     | N.D.   |       |    |          |
| T Ethylbenzene              | 9.917  | 91.0  | 389   | 0.1063 | ng    | m  | 61       |
| T m+p-Xylenes               | 10.045 | 106.0 | 0     |        | ng    | md | 1        |
| T o-Xylene                  | 0.000  |       | 0     | N.D.   |       |    |          |
| T Styrene                   | 0.000  |       | 0     | N.D.   |       |    |          |
| T Bromoform                 | 0.000  |       | 0     | N.D.   |       |    |          |
| T Bromobenzene              | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,1,2,2-Tetrachloroethane | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,2,3-Trichloropropane    | 0.000  |       | 0     | N.D.   |       |    |          |
| T 2-Chlorotoluene           | 0.000  |       | 0     | N.D.   |       |    |          |
| T 4-Chlorotoluene           | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,3-Dichlorobenzene       | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,4-Dichlorobenzene       | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,2-Dichlorobenzene       | 0.000  |       | 0     | N.D.   |       |    |          |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (\*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

# Quantitation Results Report (QT Reviewed)


| Compound                | Conc. | Exp RT | QIon | Exp Ratio |
|-------------------------|-------|--------|------|-----------|
| Dichlorodifluoromethane | N.D.  | 1.24   | 87.0 | 32.3      |




| Compound      | Conc.  | RT   | Dev(Min) | Resp.    | QIon | QRatio | Lower | Upper |
|---------------|--------|------|----------|----------|------|--------|-------|-------|
| Chloromethane | 1.4445 | 1.42 | 0.01     | 1730 (m) | 52.0 | 33.2   | 2.1   | 62.1  |



| Compound       | Conc. | Exp RT | QIon | Exp Ratio |
|----------------|-------|--------|------|-----------|
| Vinyl chloride | N.D.  | 1.50   | 64.0 | 29.9      |




| Compound     | Conc. | Exp RT | QIon | Exp Ratio |
|--------------|-------|--------|------|-----------|
| Bromomethane | N.D.  | 1.80   | 94.0 | 104.6     |




# Quantitation Results Report (QT Reviewed)


| Compound     | Conc. | Exp RT | QIon | Exp Ratio |
|--------------|-------|--------|------|-----------|
| Chloroethane | N.D.  | 1.89   | 66.0 | 30.1      |




| Compound               | Conc. | Exp RT | QIon  | Exp Ratio |
|------------------------|-------|--------|-------|-----------|
| Trichlorofluoromethane | N.D.  | 2.14   | 103.0 | 64.2      |



| Compound           | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethene | N.D.  | 2.70   | 61.0 | 180.3     | 63.0 | 56.7      |




| Compound           | Conc.  | RT   | Dev(Min) | Resp.    | QIon | QRatio | Lower | Upper |
|--------------------|--------|------|----------|----------|------|--------|-------|-------|
| Methylene chloride | 1.9869 | 3.34 | 0.00     | 2222 (m) | 84.0 | 74.8   | 36.9  | 96.9  |
|                    |        |      |          |          | 86.0 | 49.4   | 14.3  | 74.3  |




# Quantitation Results Report (QT Reviewed)


| Compound                 | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,2-Dichloroethene | N.D.  | 3.72   | 61.0 | 153.9     | 98.0 | 65.7      |




| Compound                       | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------------------|-------|--------|------|-----------|
| Methyl tert-butyl ether (MTBE) | N.D.  | 3.75   | 57.0 | 24.6      |



| Compound           | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethane | N.D.  | 4.38   | 65.0 | 32.1      | 83.0 | 13.7      |




| Compound            | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|------|-----------|
| 2,2-Dichloropropane | N.D.  | 5.20   | 41.0 | 66.5      | 97.0 | 23.2      |




# Quantitation Results Report (QT Reviewed)


| Compound               | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|------------------------|-------|--------|------|-----------|------|-----------|
| cis-1,2-Dichloroethene | N.D.  | 5.22   | 61.0 | 167.2     | 98.0 | 67.3      |




| Compound            | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| Methyl ethyl ketone | N.D.  | 5.28   | 72.0 | 21.3      |







| Compound           | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|
| Bromochloromethane | N.D.  | 5.52   | 49.0 | 182.9     |



| Compound   | Conc.  | RT   | Dev(Min) | Resp.   | QIon | QRatio | Lower | Upper |
|------------|--------|------|----------|---------|------|--------|-------|-------|
| Chloroform | 0.1455 | 5.65 | -0.01    | 209 (m) | 85.0 | 50.4   | 36.0  | 96.0  |




# Quantitation Results Report (QT Reviewed)

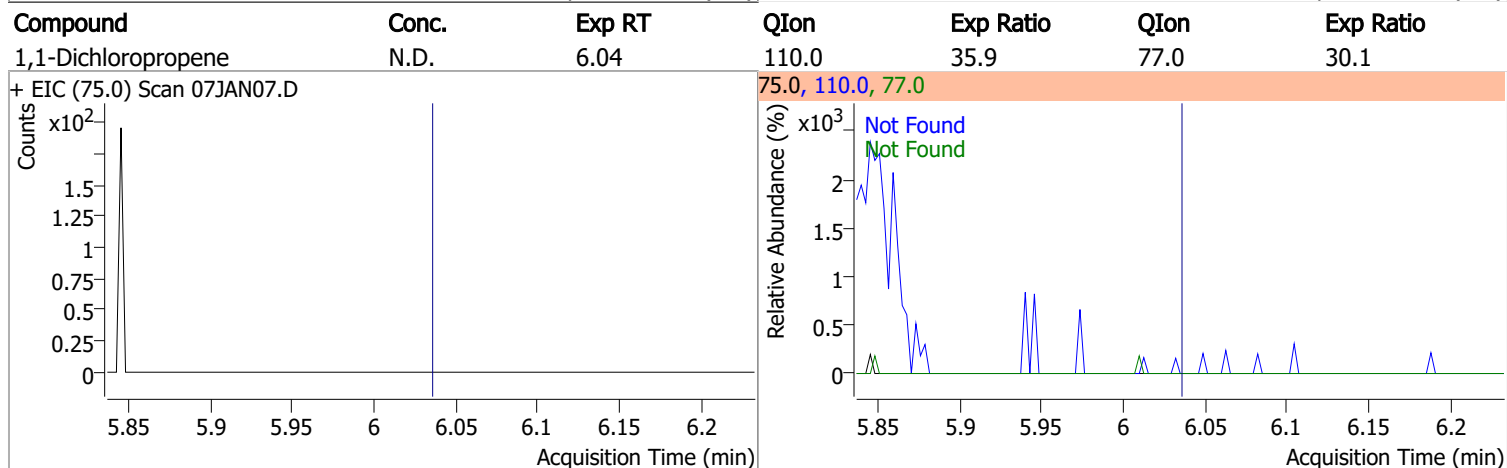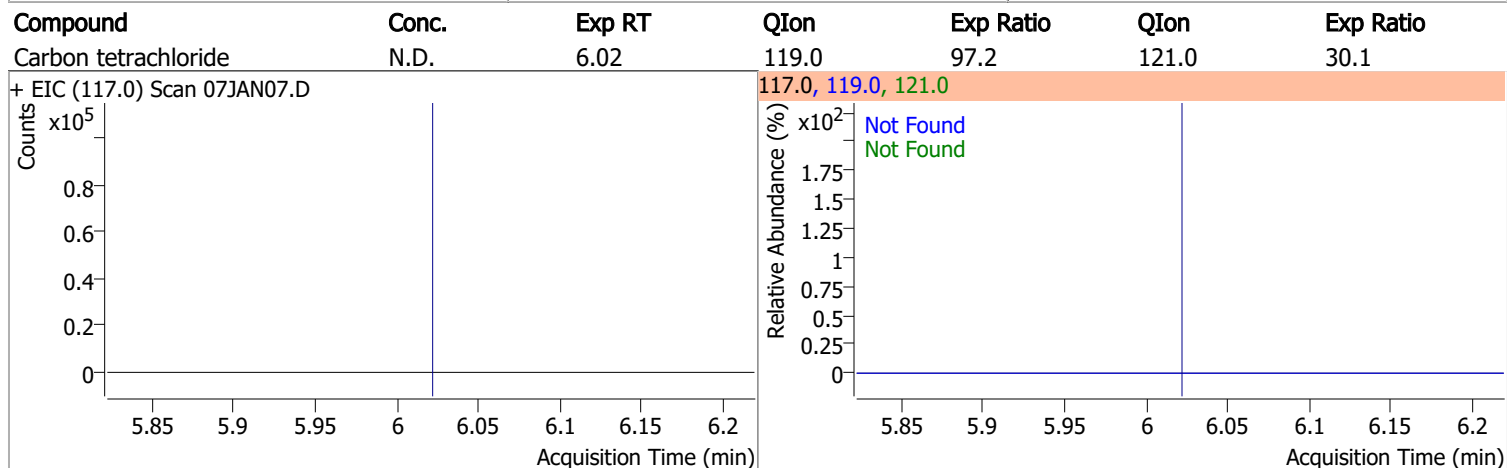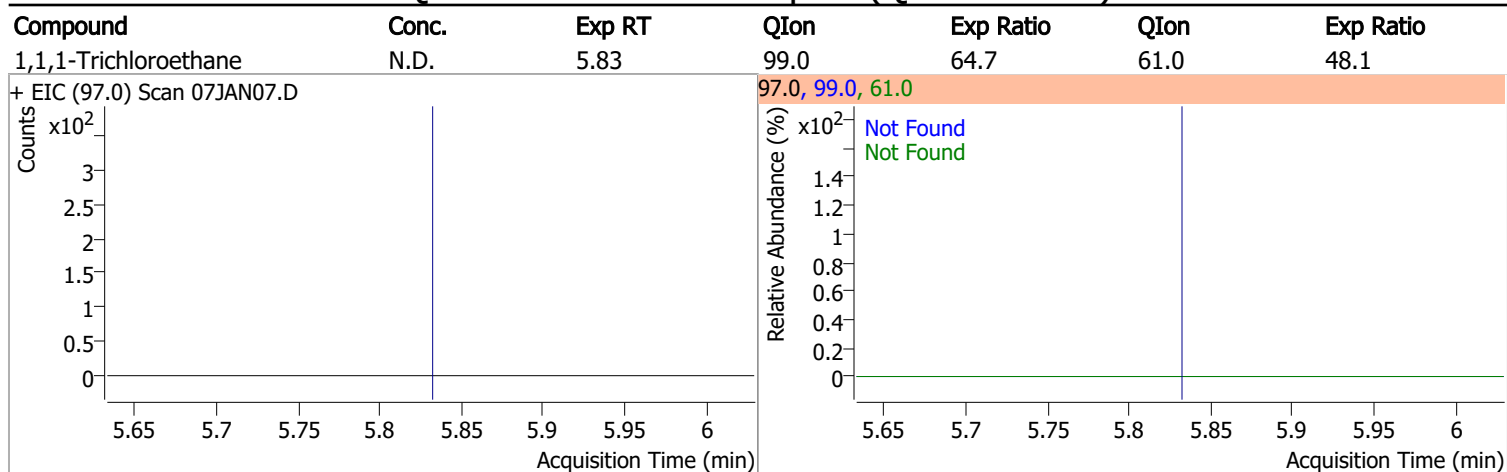


# Quantitation Results Report (QT Reviewed)


| Compound              | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 314.7549 | 6.24 | 0.00     | 96449 | 65.0 | 189.9  | 166.5 | 226.5 |

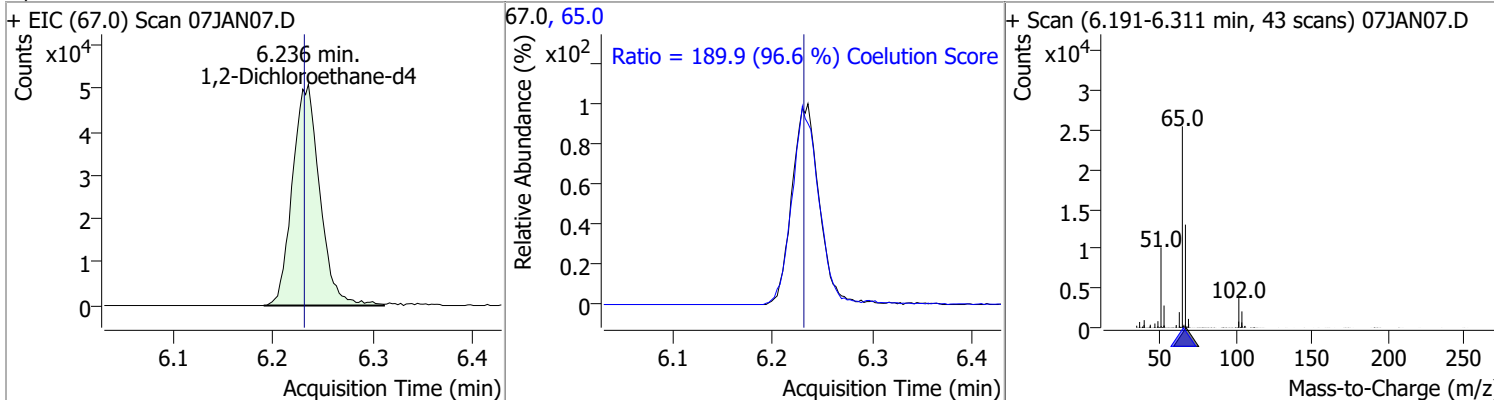


| Compound | Conc.  | RT   | Dev(Min) | Resp.   | QIon | QRatio | Lower | Upper |
|----------|--------|------|----------|---------|------|--------|-------|-------|
| Benzene  | 0.0480 | 6.29 | 0.01     | 144 (m) | 77.0 | 17.9   | 0.0   | 53.5  |











| Compound           | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,2-Dichloroethane | N.D.  | 6.32   | 64.0 | 29.9      | 98.0 | 7.6       |

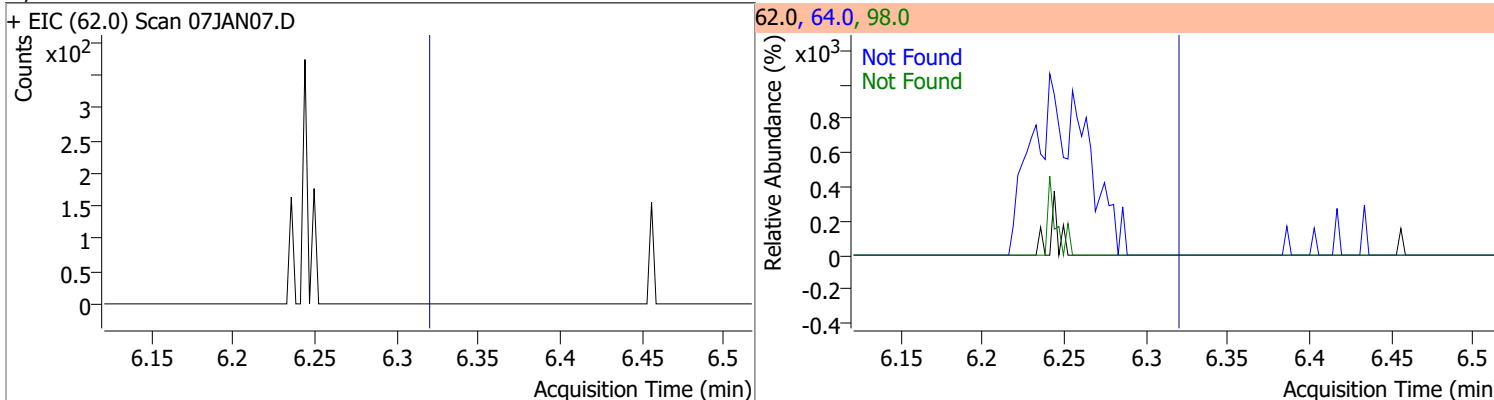

| Compound        | Conc. | Exp RT | QIon  | Exp Ratio | QIon | Exp Ratio |
|-----------------|-------|--------|-------|-----------|------|-----------|
| Trichloroethene | N.D.  | 7.03   | 130.0 | 101.5     | 97.0 | 64.1      |

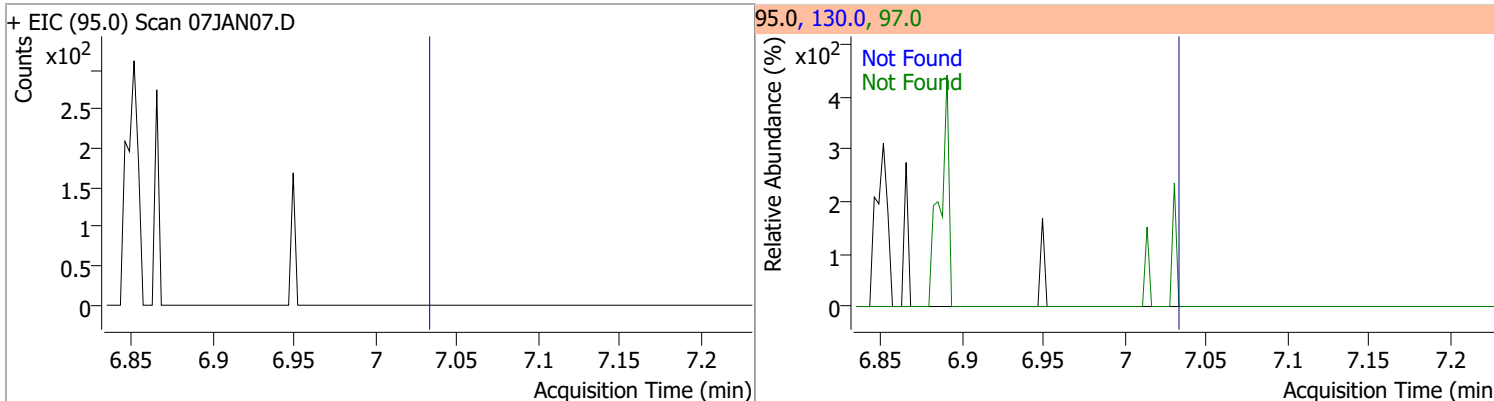


# Quantitation Results Report (QT Reviewed)
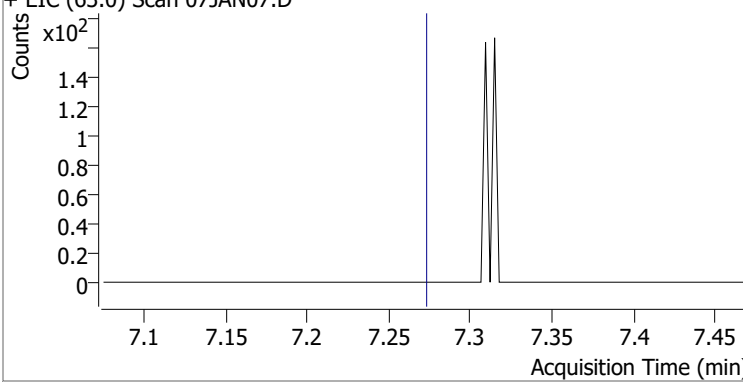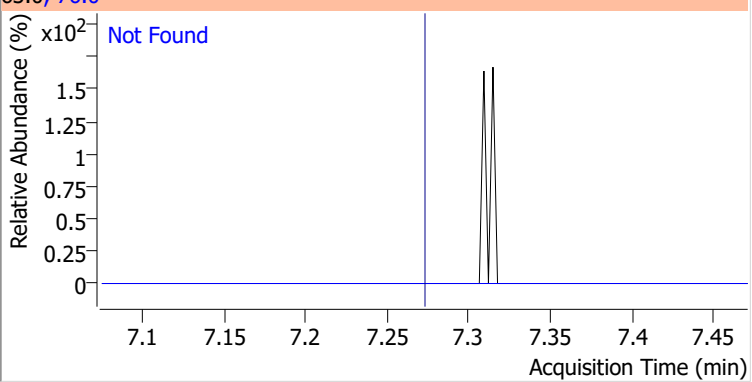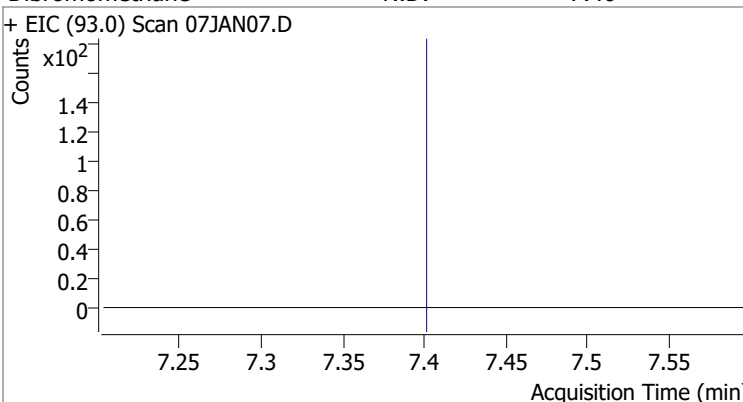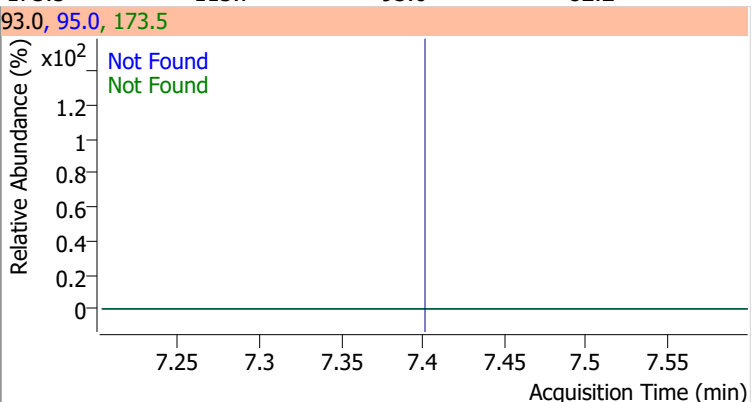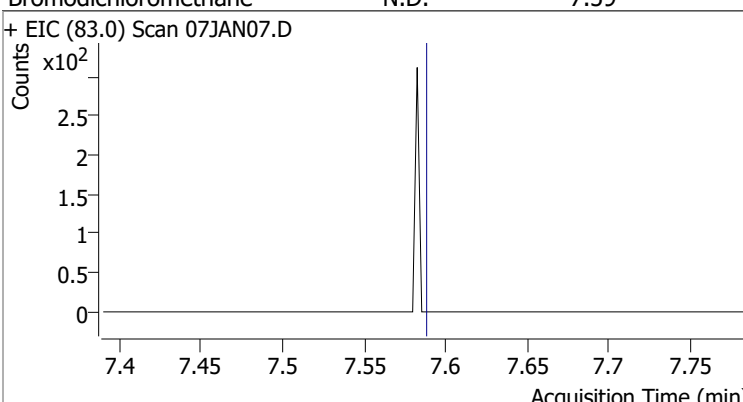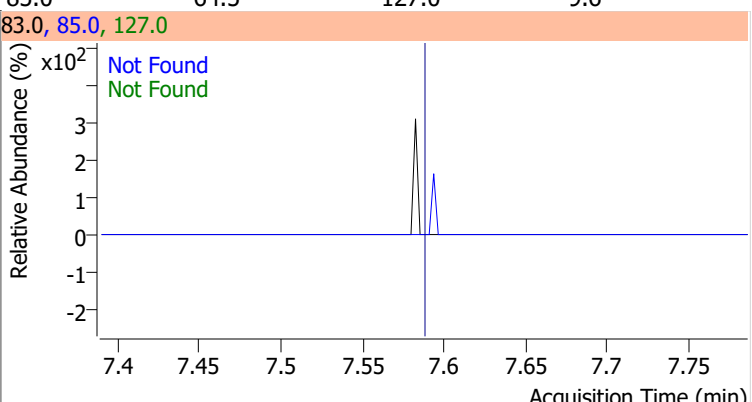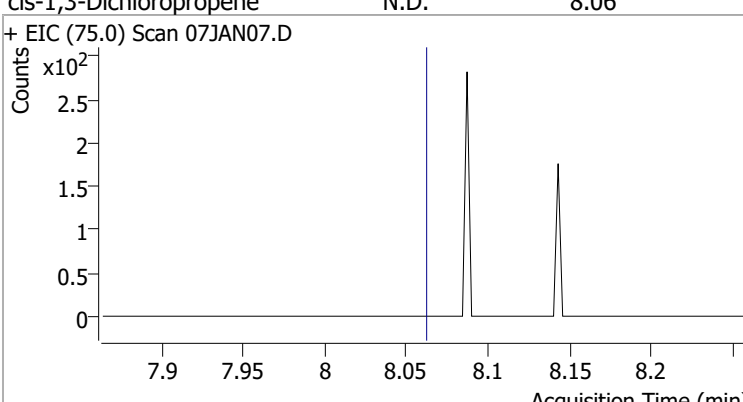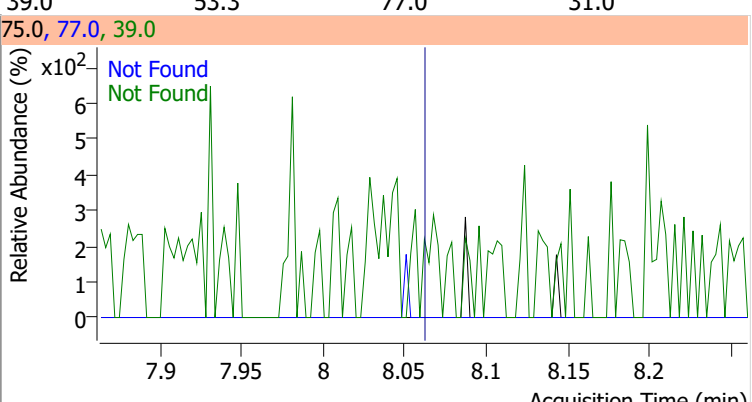
| Compound                                                                           | Conc. | Exp RT | QIon                                                                                 | Exp Ratio |      |           |
|------------------------------------------------------------------------------------|-------|--------|--------------------------------------------------------------------------------------|-----------|------|-----------|
| 1,2-Dichloropropane                                                                | N.D.  | 7.27   | 76.0                                                                                 | 38.2      |      |           |
| + EIC (63.0) Scan 07JAN07.D                                                        |       |        | 63.0, 76.0                                                                           |           |      |           |
|    |       |        |    |           |      |           |
| Dibromomethane                                                                     | N.D.  | 7.40   | 173.5                                                                                | 113.7     | QIon | Exp Ratio |
| + EIC (93.0) Scan 07JAN07.D                                                        |       |        | 93.0, 95.0, 173.5                                                                    |           |      |           |
|   |       |        |   |           |      |           |
| Bromodichloromethane                                                               | N.D.  | 7.59   | 85.0                                                                                 | 64.5      | QIon | Exp Ratio |
| + EIC (83.0) Scan 07JAN07.D                                                        |       |        | 83.0, 85.0, 127.0                                                                    |           |      |           |
|  |       |        |  |           |      |           |
| cis-1,3-Dichloropropene                                                            | N.D.  | 8.06   | 39.0                                                                                 | 53.3      | QIon | Exp Ratio |
| + EIC (75.0) Scan 07JAN07.D                                                        |       |        | 75.0, 77.0, 39.0                                                                     |           |      |           |
|  |       |        |  |           |      |           |




# Quantitation Results Report (QT Reviewed)


| Compound   | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 260.0307 | 8.32 | 0.00     | 740894 | 100.0 | 64.5   | 34.4  | 94.4  |
|            |          |      |          |        | 99.0  | 9.5    | 0.0   | 39.6  |

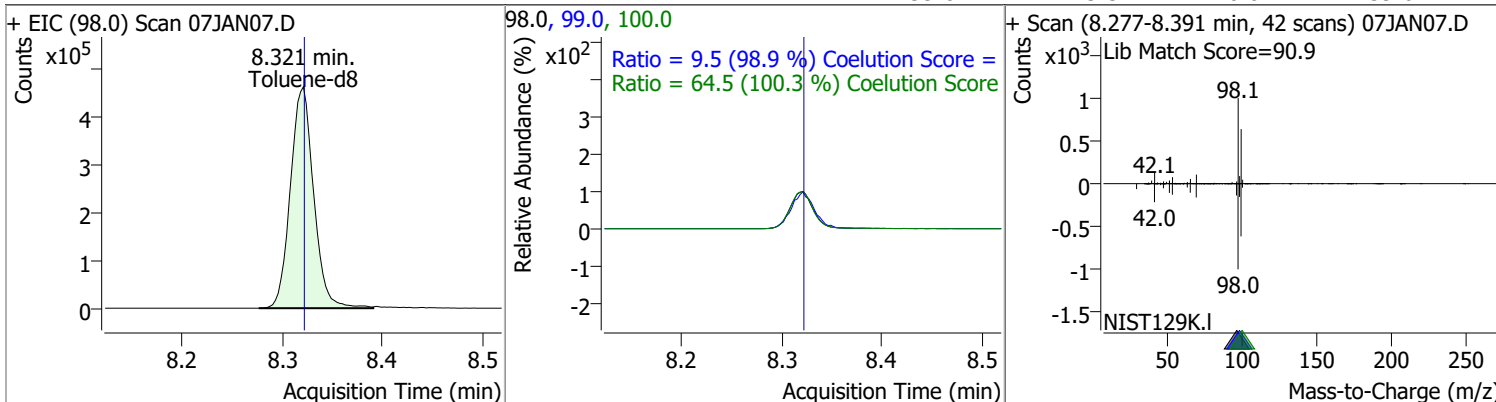


| Compound | Conc.  | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|--------|------|----------|-------|------|--------|-------|-------|
| Toluene  | 1.9977 | 8.39 | 0.00     | 3845  | 91.0 | 175.2  | 145.8 | 205.8 |

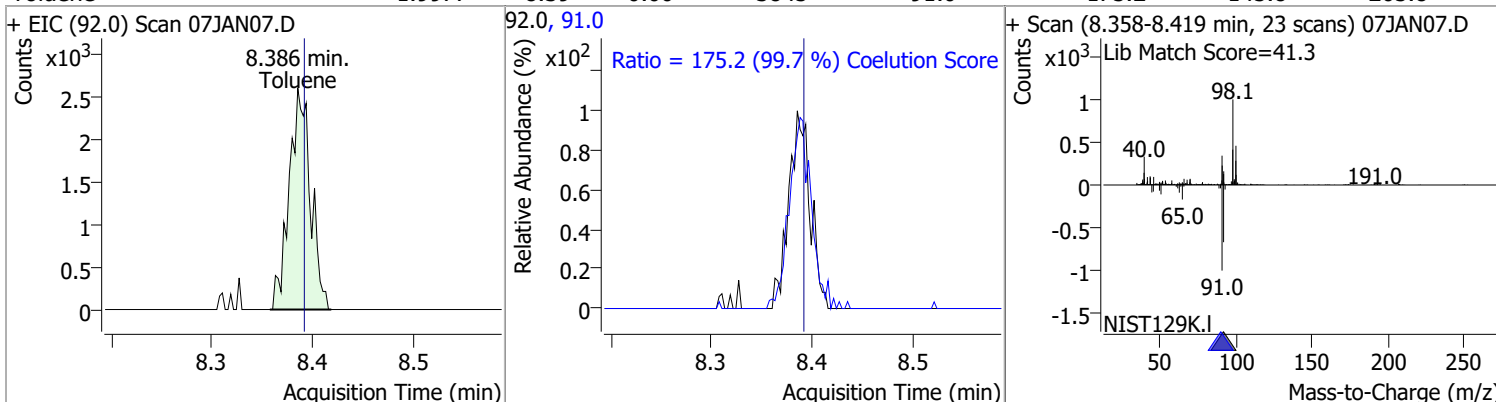

| Compound                  | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,3-Dichloropropene | N.D.  | 8.64   | 39.0 | 53.4      | 77.0 | 32.4      |

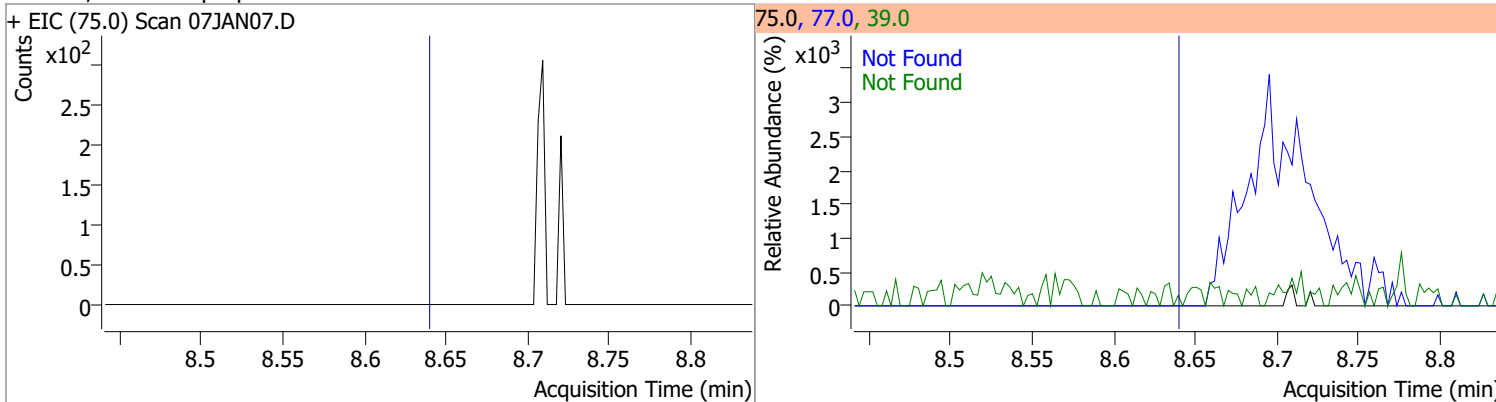





| Compound              | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------------|-------|--------|------|-----------|------|-----------|
| 1,1,2-Trichloroethane | N.D.  | 8.82   | 97.0 | 114.6     | 85.0 | 67.6      |

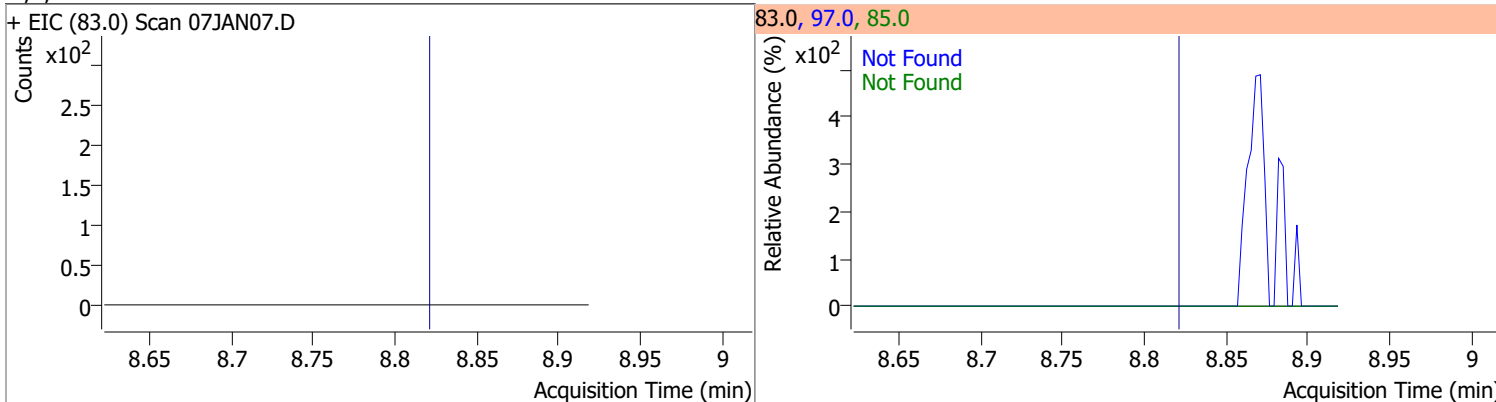

# Quantitation Results Report (QT Reviewed)


| Compound                                          | Conc. | Exp RT | QIon                | Exp Ratio | QIon  | Exp Ratio |
|---------------------------------------------------|-------|--------|---------------------|-----------|-------|-----------|
| Tetrachloroethene                                 | N.D.  | 8.94   | 165.8               | 128.6     | 129.0 | 91.5      |
| + EIC (163.8) Scan 07JAN07.D ***NO DATA POINTS*** |       |        | 163.8, 129.0, 165.8 |           |       |           |
|                                                   |       |        |                     |           |       |           |
| 1,3-Dichloropropane                               | N.D.  | 8.98   | 78.0                | 32.9      |       |           |
| + EIC (76.0) Scan 07JAN07.D                       |       |        | 76.0, 78.0          |           |       |           |
|                                                   |       |        |                     |           |       |           |
| Chlorodibromomethane                              | N.D.  | 9.21   | 127.0               | 78.0      |       |           |
| + EIC (129.0) Scan 07JAN07.D ***NO DATA POINTS*** |       |        | 129.0, 127.0        |           |       |           |
|                                                   |       |        |                     |           |       |           |
| 1,2-Dibromoethane                                 | N.D.  | 9.31   | 109.0               | 94.5      |       |           |
| + EIC (107.0) Scan 07JAN07.D                      |       |        | 107.0, 109.0        |           |       |           |
|                                                   |       |        |                     |           |       |           |

# Quantitation Results Report (QT Reviewed)

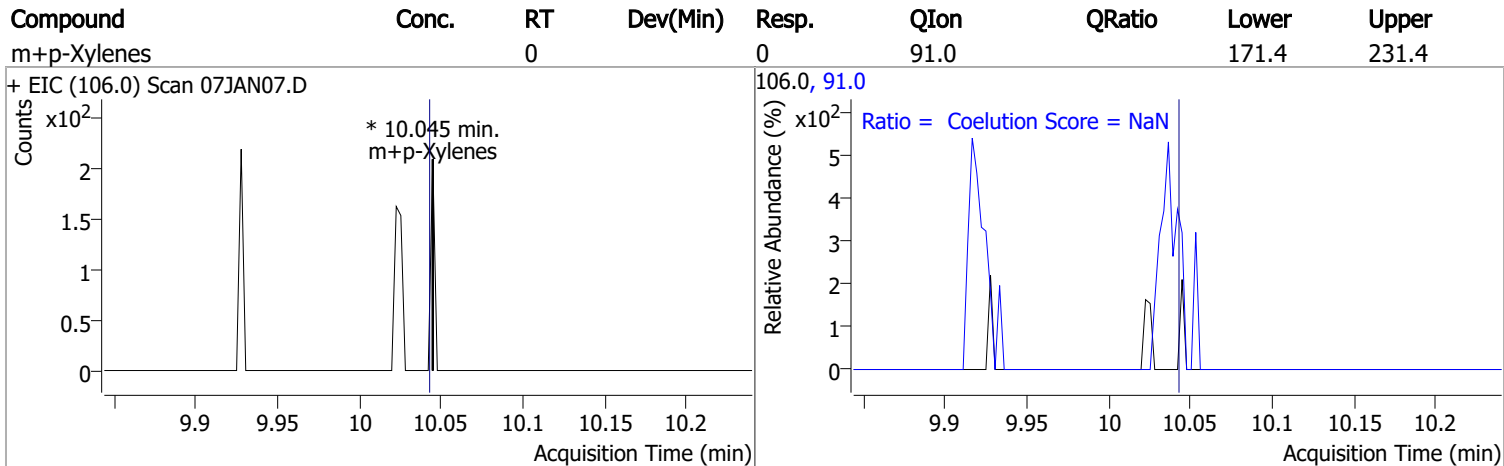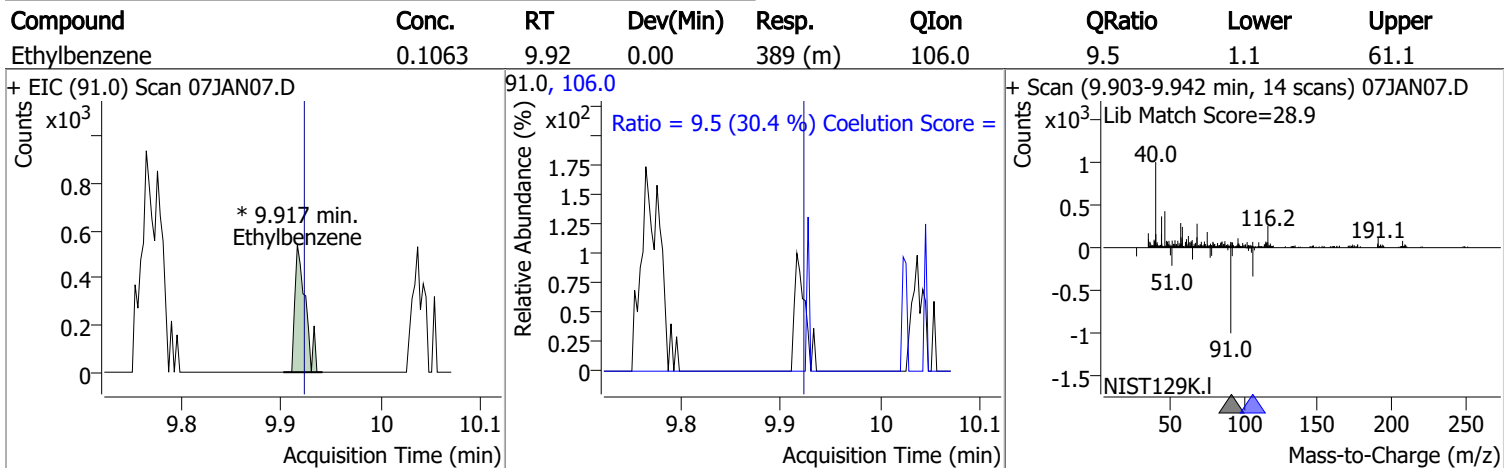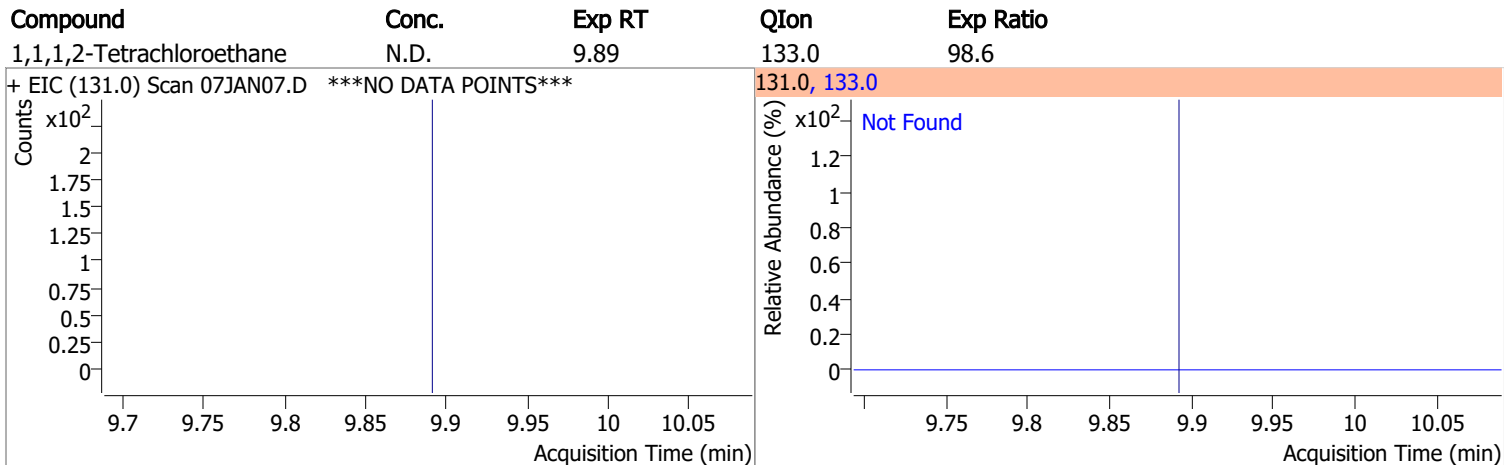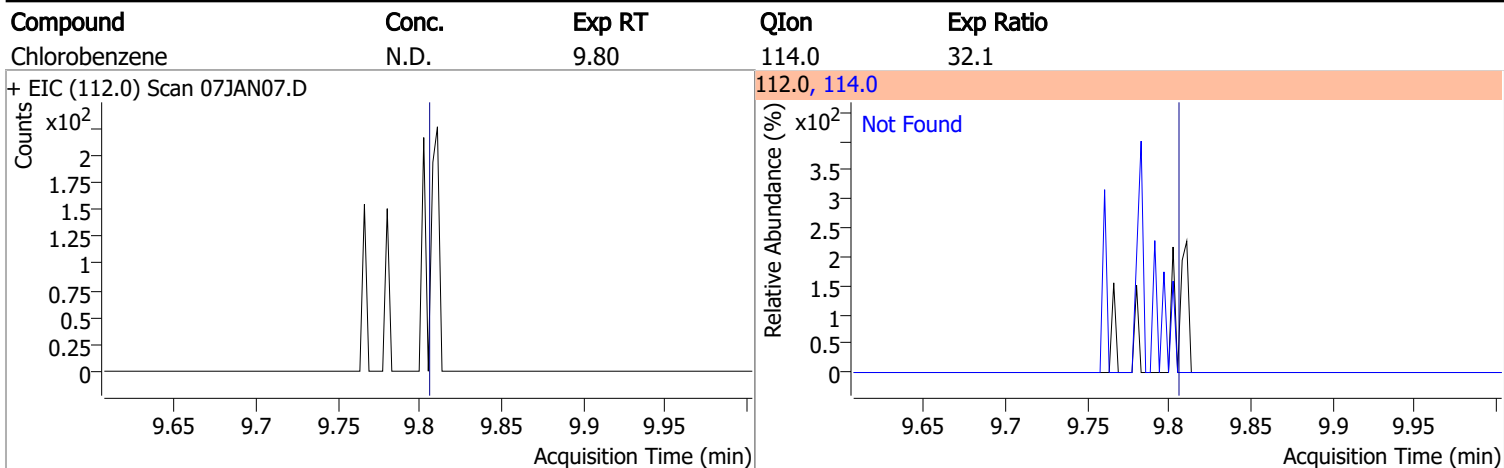


# Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------|-------|--------|------|-----------|
| o-Xylene | N.D.  | 10.43  | 91.0 | 213.1     |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------|-------|--------|------|-----------|
| Styrene  | N.D.  | 10.45  | 78.0 | 49.6      |











| Compound  | Conc. | Exp RT | QIon  | Exp Ratio | QIon  | Exp Ratio |
|-----------|-------|--------|-------|-----------|-------|-----------|
| Bromoform | N.D.  | 10.63  | 170.5 | 52.1      | 174.5 | 50.1      |











| Compound             | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 283.5551 | 10.95 | 0.00     | 215644 | 174.0 | 93.3   | 61.7  | 121.7 |
|                      |          |       |          |        | 176.0 | 91.4   | 60.6  | 120.6 |



# Quantitation Results Report (QT Reviewed)

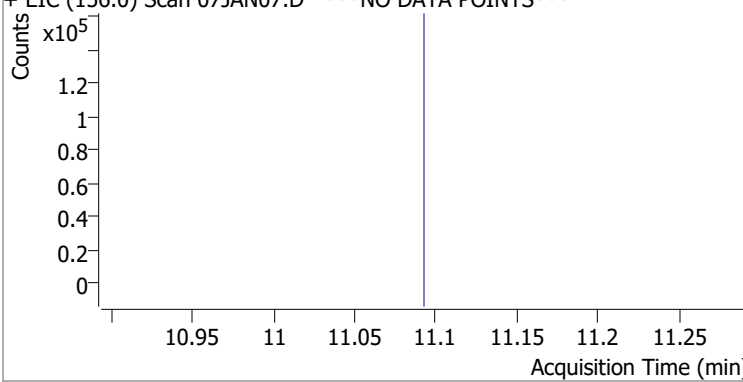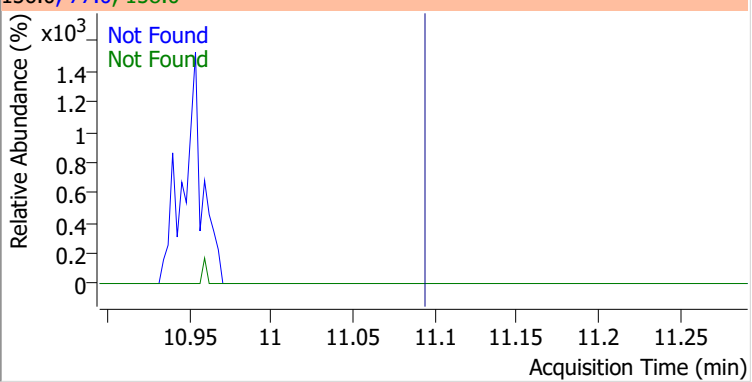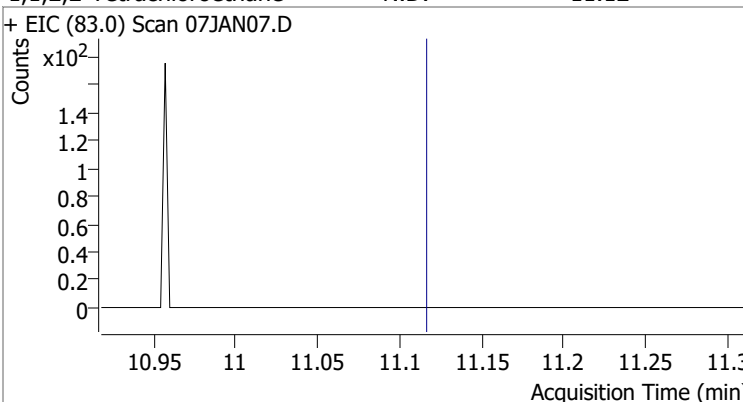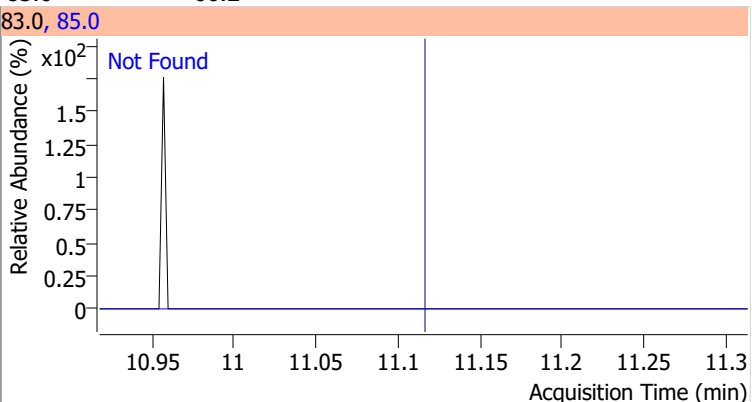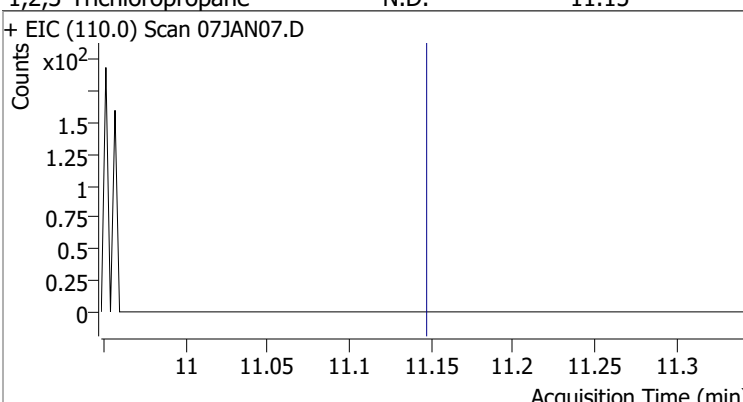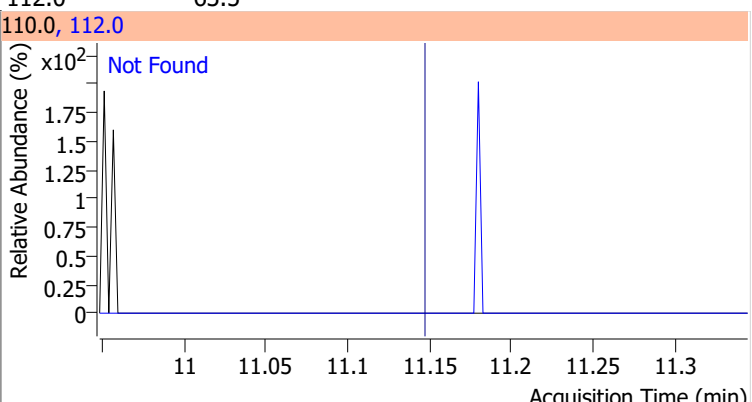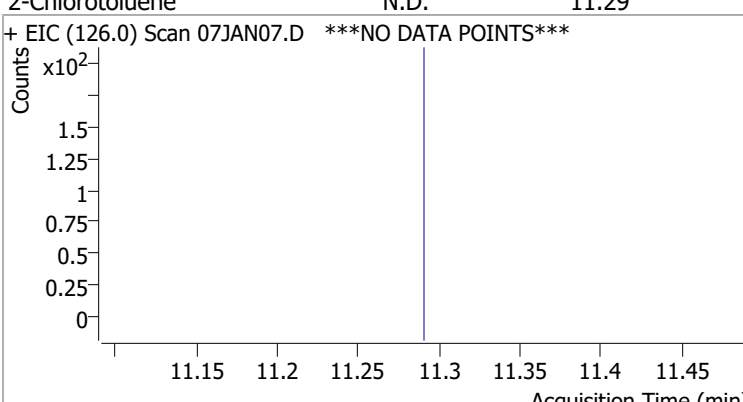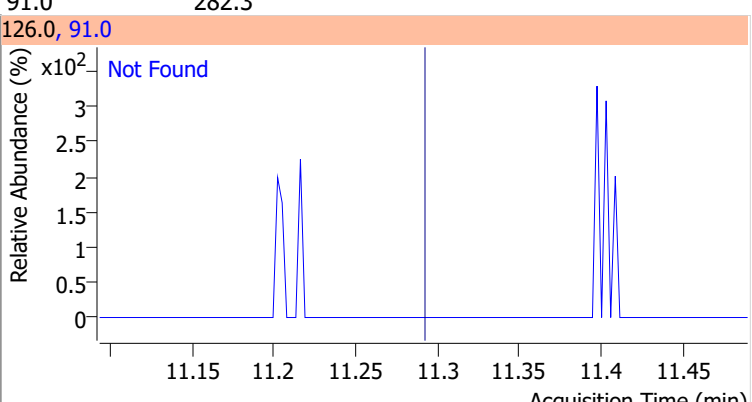
| Compound                                                                           | Conc. | Exp RT | QIon                                                                                 | Exp Ratio | QIon  | Exp Ratio |
|------------------------------------------------------------------------------------|-------|--------|--------------------------------------------------------------------------------------|-----------|-------|-----------|
| Bromobenzene                                                                       | N.D.  | 11.09  | 77.0                                                                                 | 145.7     | 158.0 | 96.5      |
| + EIC (156.0) Scan 07JAN07.D ***NO DATA POINTS***                                  |       |        | 156.0, 77.0, 158.0                                                                   |           |       |           |
|    |       |        |    |           |       |           |
| 1,1,2-Tetrachloroethane                                                            | N.D.  | 11.12  | 85.0                                                                                 | 66.2      |       |           |
| + EIC (83.0) Scan 07JAN07.D                                                        |       |        | 83.0, 85.0                                                                           |           |       |           |
|   |       |        |   |           |       |           |
| 1,2,3-Trichloropropane                                                             | N.D.  | 11.15  | 112.0                                                                                | 63.5      |       |           |
| + EIC (110.0) Scan 07JAN07.D                                                       |       |        | 110.0, 112.0                                                                         |           |       |           |
|  |       |        |  |           |       |           |
| 2-Chlorotoluene                                                                    | N.D.  | 11.29  | 91.0                                                                                 | 282.3     |       |           |
| + EIC (126.0) Scan 07JAN07.D ***NO DATA POINTS***                                  |       |        | 126.0, 91.0                                                                          |           |       |           |
|  |       |        |  |           |       |           |

# Quantitation Results Report (QT Reviewed)
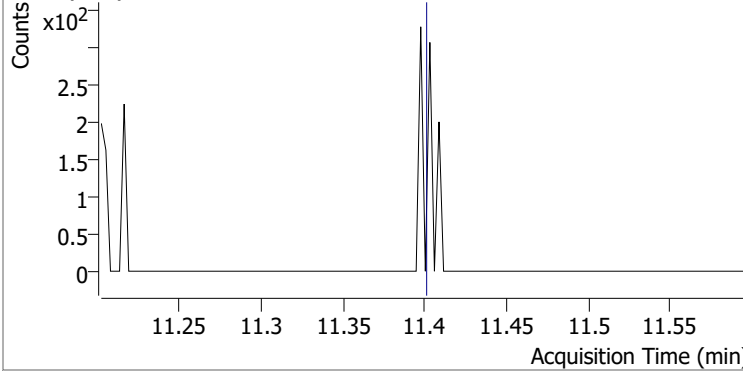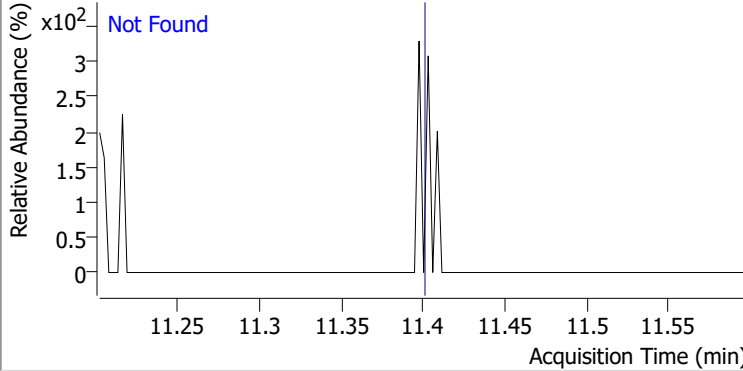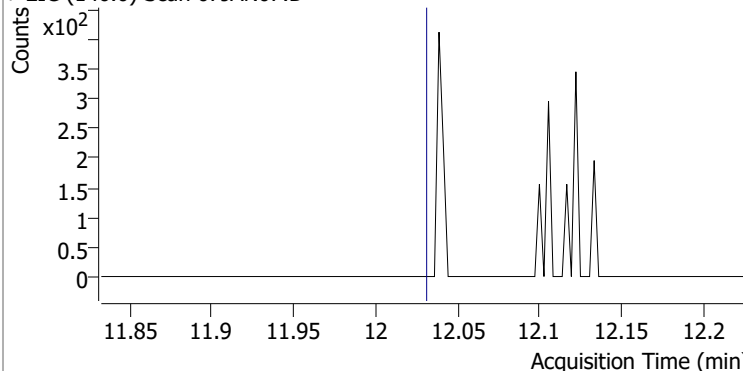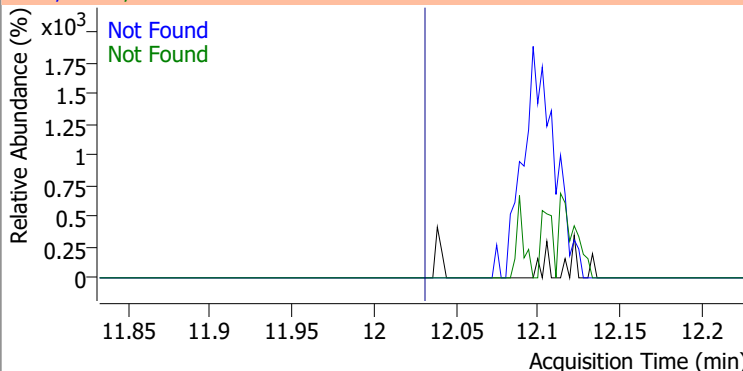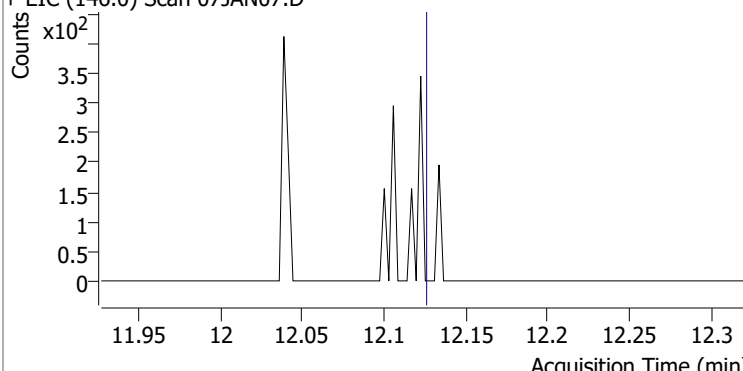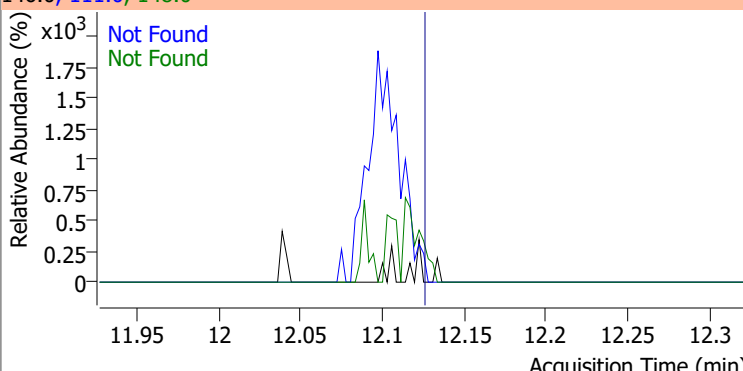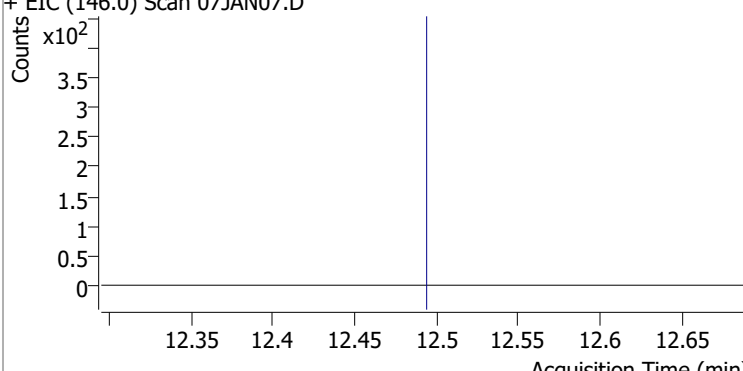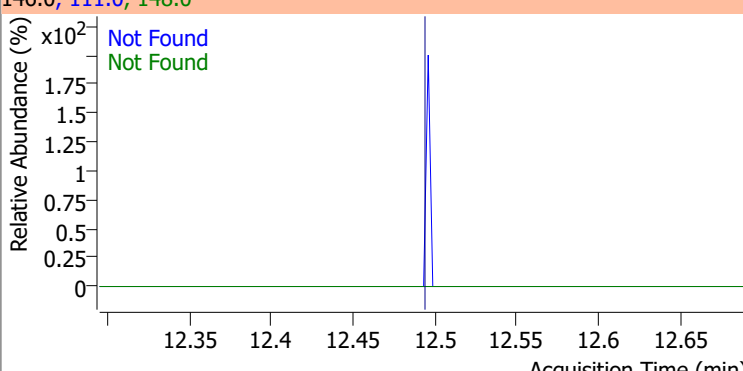
| Compound                     | Conc. | Exp RT | QIon                                                                                 | Exp Ratio | QIon        | Exp Ratio |
|------------------------------|-------|--------|--------------------------------------------------------------------------------------|-----------|-------------|-----------|
| 4-Chlorotoluene              | N.D.  | 11.40  | 126.0                                                                                | 31.7      | 91.0, 126.0 |           |
| + EIC (91.0) Scan 07JAN07.D  |       |        |      |           |             |           |
|                              |       |        |    |           |             |           |
| 1,3-Dichlorobenzene          | N.D.  | 12.03  | 148.0                                                                                | 63.6      | 111.0       | 39.8      |
| + EIC (146.0) Scan 07JAN07.D |       |        |     |           |             |           |
|                              |       |        |   |           |             |           |
| 1,4-Dichlorobenzene          | N.D.  | 12.13  | 148.0                                                                                | 63.1      | 111.0       | 39.1      |
| + EIC (146.0) Scan 07JAN07.D |       |        |    |           |             |           |
|                              |       |        |  |           |             |           |
| 1,2-Dichlorobenzene          | N.D.  | 12.49  | 148.0                                                                                | 63.9      | 111.0       | 41.0      |
| + EIC (146.0) Scan 07JAN07.D |       |        |    |           |             |           |
|                              |       |        |  |           |             |           |

# Quantitation Results Report (QT Reviewed)

|                |                                     |                   |                       |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File      | 07JAN08.D                           | Operator          | MSC                   |
| Acq. Method    | 5975CACQF.M                         | Acq. Date-Time    | 1/7/2022 12:52:15 PM  |
| Sample Name    | B22010219-002A                      | Instrument        | VOA5975C              |
| Vial           | 8                                   | Multiplier        | 1.00                  |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m  | Comment           |                       |
| Tune File      | BFB_Atune3.u                        | Tune Date         | 10/11/2021 4:02:00 PM |
| Batch Name     | VG010722_8260B.batch.bin            | Last Calib Update | 3/2/2022 10:41:44 AM  |
| Ref Library    | \\MASSHUNTER\Org\Library\NIST129K.I |                   |                       |



| Compound                           | RT                   | QIon  | Resp.  | Conc.              | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|--------------------|-------|----------|
| <b>Internal Standards</b>          |                      |       |        |                    |       |          |
| M Fluorobenzene                    | 6.618                | 96.0  | 819676 | 250.0000           | ng    | -0.006   |
| M Chlorobenzene-d5                 | 9.772                | 82.0  | 322006 | 250.0000           | ng    | 0.000    |
| M 1,4-Dichlorobenzene-d4           | 12.100               | 152.0 | 235354 | 250.0000           | ng    | 0.000    |
| <b>System Monitoring Compounds</b> |                      |       |        |                    |       |          |
| S Dibromofluoromethane             | 5.848                | 113.0 | 212882 | 275.6761           | ng    | 0.003    |
| Spiked Amount: 250.000             | Range: 80.0 - 119.0% |       |        | Recovery = 110.27% |       |          |
| S 1,2-Dichloroethane-d4            | 6.233                | 67.0  | 96571  | 289.5314           | ng    | 0.000    |
| Spiked Amount: 250.000             | Range: 81.0 - 118.0% |       |        | Recovery = 115.81% |       |          |
| S Toluene-d8                       | 8.319                | 98.0  | 818871 | 263.8953           | ng    | 0.000    |
| Spiked Amount: 250.000             | Range: 89.0 - 112.0% |       |        | Recovery = 105.56% |       |          |
| S p-Bromofluorobenzene             | 10.951               | 95.0  | 240793 | 279.2702           | ng    | -0.003   |
| Spiked Amount: 250.000             | Range: 85.0 - 114.0% |       |        | Recovery = 111.71% |       |          |
| <b>Target Compounds</b>            |                      |       |        |                    |       |          |
| T Dichlorodifluoromethane          | 0.000                |       | 0      | N.D.               |       |          |
| T Chloromethane                    | 1.406                | 50.0  | 2485   | 1.9061             | ng    | 96       |
| T Vinyl chloride                   | 0.000                |       | 0      | N.D.               |       |          |
| T Bromomethane                     | 0.000                |       | 0      | N.D.               |       |          |
| T Chloroethane                     | 0.000                |       | 0      | N.D.               |       |          |
| T Trichlorofluoromethane           | 0.000                |       | 0      | N.D.               |       |          |
| T 1,1-Dichloroethene               | 0.000                |       | 0      | N.D.               |       |          |
| T Methylene chloride               | 3.333                | 49.0  | 2231   | 1.8330             | ng    | 97       |
| T trans-1,2-Dichloroethene         | 0.000                |       | 0      | N.D.               |       |          |
| T Methyl tert-butyl ether (MTBE)   | 0.000                |       | 0      | N.D.               |       |          |
| T 1,1-Dichloroethane               | 0.000                |       | 0      | N.D.               |       |          |
| T 2,2-Dichloropropane              | 0.000                |       | 0      | N.D.               |       |          |
| T cis-1,2-Dichloroethene           | 0.000                |       | 0      | N.D.               |       |          |
| T Methyl ethyl ketone              | 0.000                |       | 0      | N.D.               |       |          |
| T Bromochloromethane               | 0.000                |       | 0      | N.D.               |       |          |
| T Chloroform                       | 0.000                |       | 0      | N.D.               |       |          |

# Quantitation Results Report (QT Reviewed)


| Compound                    | RT     | QIon  | Resp. | Conc.  | Units |    | Dev(Min) |
|-----------------------------|--------|-------|-------|--------|-------|----|----------|
| T 1,1,1-Trichloroethane     | 0.000  |       | 0     | N.D.   |       |    |          |
| T Carbon tetrachloride      | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,1-Dichloropropene       | 0.000  |       | 0     | N.D.   |       |    |          |
| T Benzene                   | 6.275  | 78.0  | 212   | 0.0648 | ng    | m  | 67       |
| T 1,2-Dichloroethane        | 0.000  |       | 0     | N.D.   |       |    |          |
| T Trichloroethene           | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,2-Dichloropropane       | 0.000  |       | 0     | N.D.   |       |    |          |
| T Dibromomethane            | 0.000  |       | 0     | N.D.   |       |    |          |
| T Bromodichloromethane      | 0.000  |       | 0     | N.D.   |       |    |          |
| T cis-1,3-Dichloropropene   | 0.000  |       | 0     | N.D.   |       |    |          |
| T Toluene                   | 8.388  | 92.0  | 3792  | 1.8091 | ng    |    | 95       |
| T trans-1,3-Dichloropropene | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,1,2-Trichloroethane     | 0.000  |       | 0     | N.D.   |       |    |          |
| T Tetrachloroethene         | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,3-Dichloropropane       | 0.000  |       | 0     | N.D.   |       |    |          |
| T Chlorodibromomethane      | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,2-Dibromoethane         | 0.000  |       | 0     | N.D.   |       |    |          |
| T Chlorobenzene             | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,1,1,2-Tetrachloroethane | 0.000  |       | 0     | N.D.   |       |    |          |
| T Ethylbenzene              | 9.911  | 91.0  | 483   | 0.1214 | ng    | m  | 53       |
| T m+p-Xylenes               | 10.037 | 106.0 | 0     |        | ng    | md | 1        |
| T o-Xylene                  | 0.000  |       | 0     | N.D.   |       |    |          |
| T Styrene                   | 0.000  |       | 0     | N.D.   |       |    |          |
| T Bromoform                 | 0.000  |       | 0     | N.D.   |       |    |          |
| T Bromobenzene              | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,1,2,2-Tetrachloroethane | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,2,3-Trichloropropane    | 0.000  |       | 0     | N.D.   |       |    |          |
| T 2-Chlorotoluene           | 0.000  |       | 0     | N.D.   |       |    |          |
| T 4-Chlorotoluene           | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,3-Dichlorobenzene       | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,4-Dichlorobenzene       | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,2-Dichlorobenzene       | 0.000  |       | 0     | N.D.   |       |    |          |

(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (\*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak




# Quantitation Results Report (QT Reviewed)


| Compound                | Conc. | Exp RT | QIon | Exp Ratio |
|-------------------------|-------|--------|------|-----------|
| Dichlorodifluoromethane | N.D.  | 1.24   | 87.0 | 32.3      |

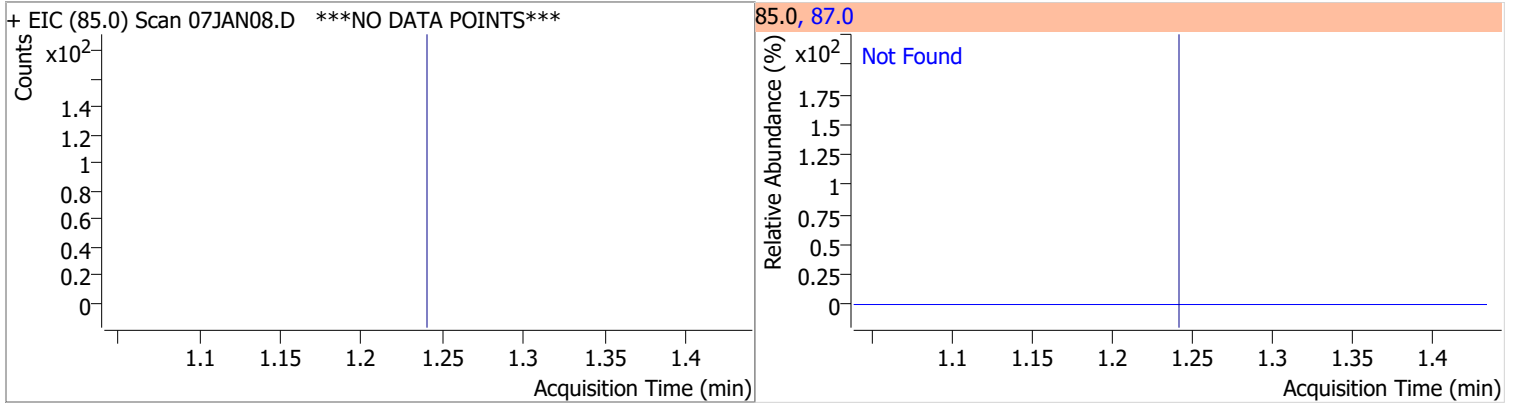


| Compound      | Conc.  | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------|--------|------|----------|-------|------|--------|-------|-------|
| Chloromethane | 1.9061 | 1.41 | 0.00     | 2485  | 52.0 | 29.7   | 2.1   | 62.1  |

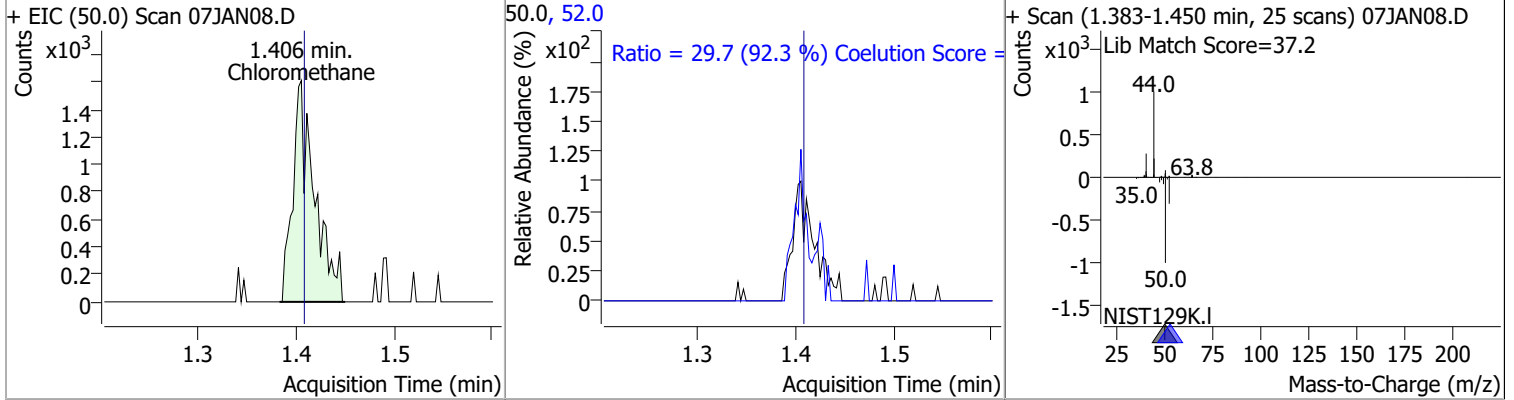

| Compound       | Conc. | Exp RT | QIon | Exp Ratio |
|----------------|-------|--------|------|-----------|
| Vinyl chloride | N.D.  | 1.50   | 64.0 | 29.9      |

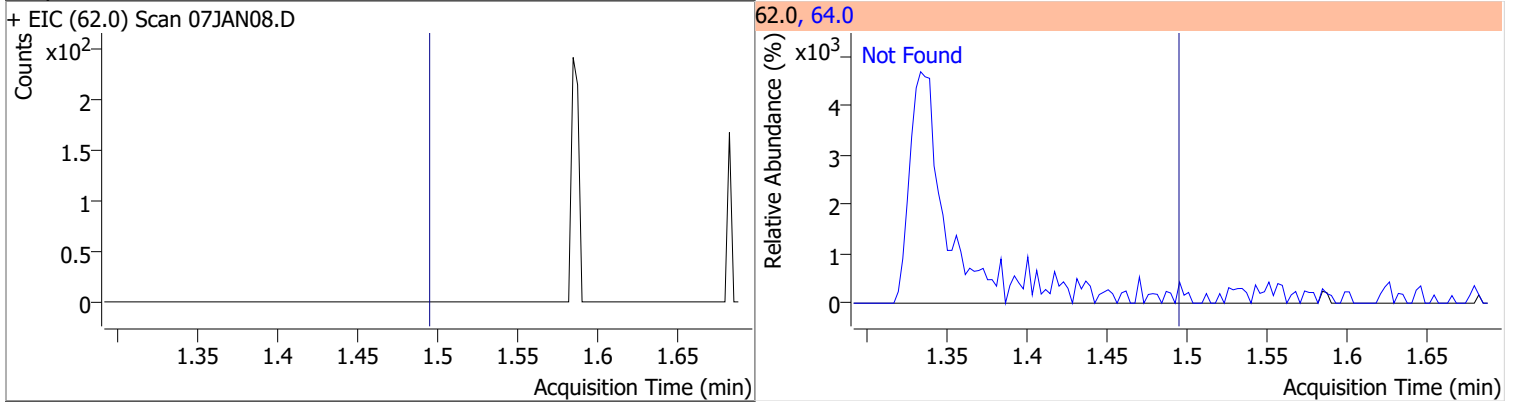


| Compound     | Conc. | Exp RT | QIon | Exp Ratio |
|--------------|-------|--------|------|-----------|
| Bromomethane | N.D.  | 1.80   | 94.0 | 104.6     |

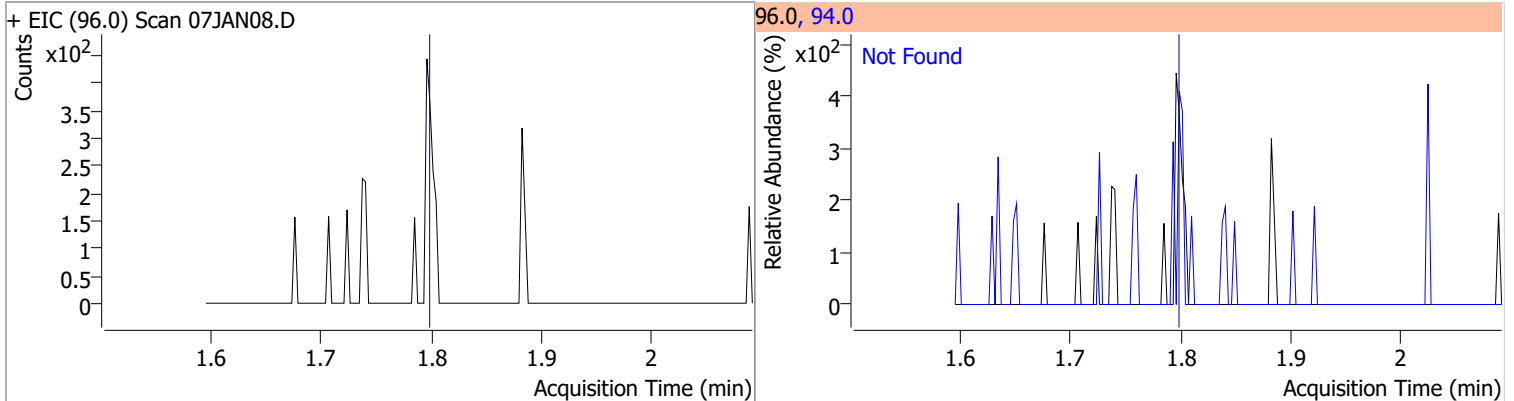


# Quantitation Results Report (QT Reviewed)


| Compound     | Conc. | Exp RT | QIon | Exp Ratio |
|--------------|-------|--------|------|-----------|
| Chloroethane | N.D.  | 1.89   | 66.0 | 30.1      |

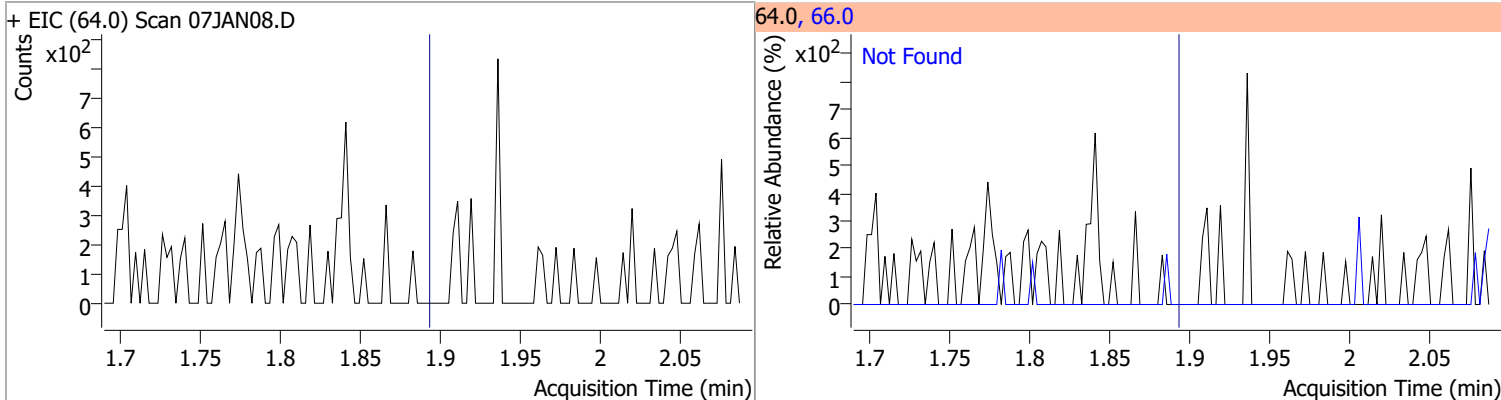


| Compound               | Conc. | Exp RT | QIon  | Exp Ratio |
|------------------------|-------|--------|-------|-----------|
| Trichlorofluoromethane | N.D.  | 2.14   | 103.0 | 64.2      |

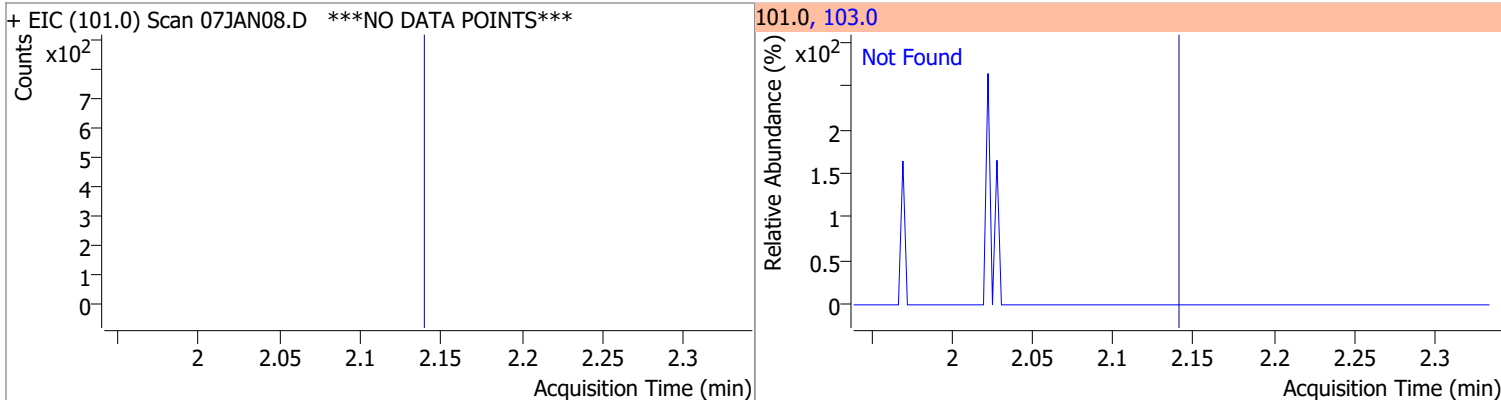

| Compound           | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethene | N.D.  | 2.70   | 61.0 | 180.3     | 63.0 | 56.7      |

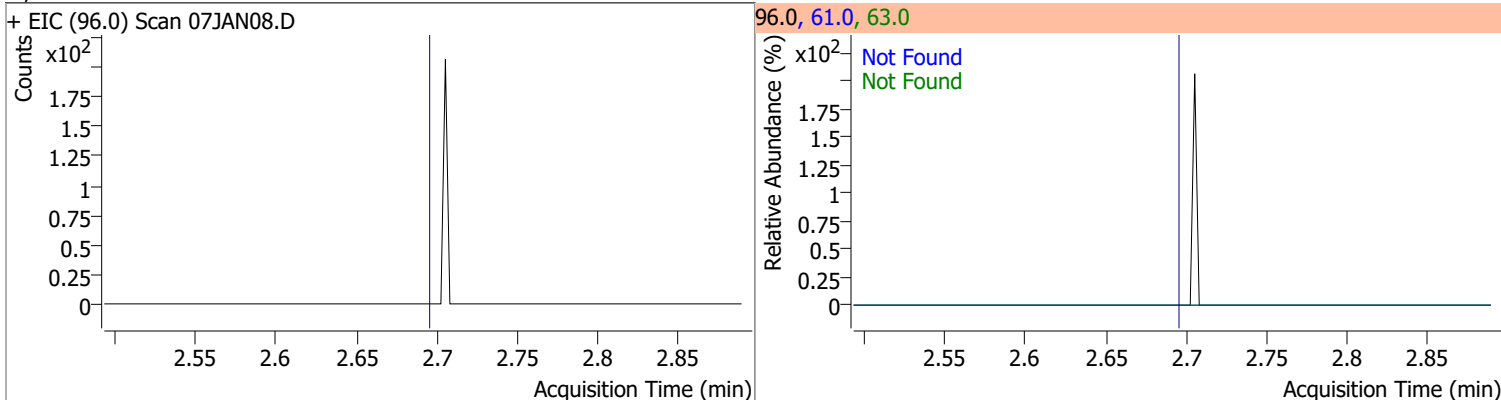


| Compound           | Conc.  | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|--------|------|----------|-------|------|--------|-------|-------|
| Methylene chloride | 1.8330 | 3.33 | 0.00     | 2231  | 84.0 | 70.2   | 36.9  | 96.9  |
|                    |        |      |          |       | 86.0 | 43.8   | 14.3  | 74.3  |

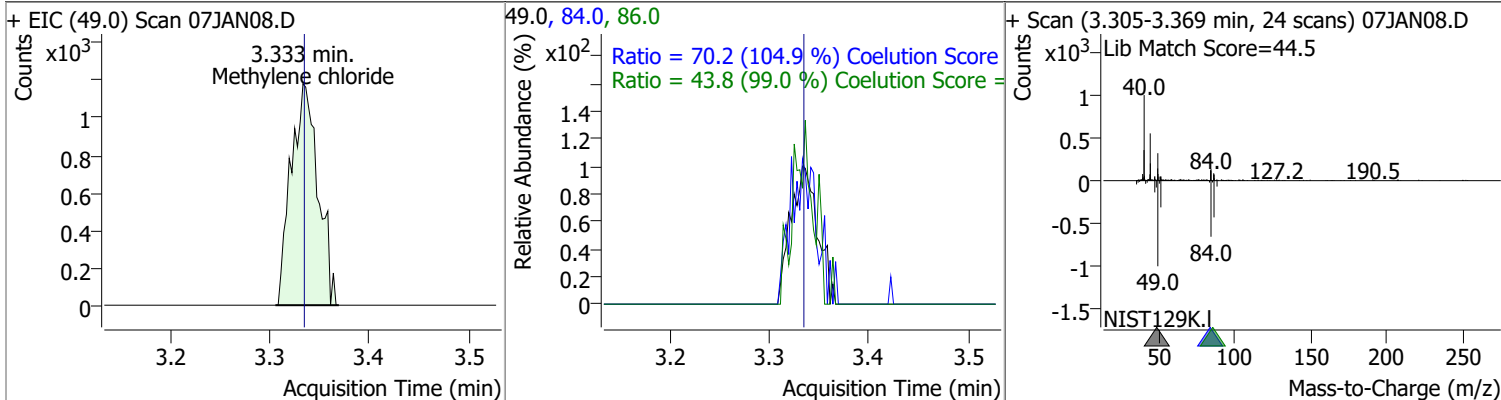


# Quantitation Results Report (QT Reviewed)


| Compound                 | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,2-Dichloroethene | N.D.  | 3.72   | 61.0 | 153.9     | 98.0 | 65.7      |




| Compound                       | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------------------|-------|--------|------|-----------|
| Methyl tert-butyl ether (MTBE) | N.D.  | 3.75   | 57.0 | 24.6      |











| Compound           | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethane | N.D.  | 4.38   | 65.0 | 32.1      | 83.0 | 13.7      |



| Compound            | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|------|-----------|
| 2,2-Dichloropropane | N.D.  | 5.20   | 41.0 | 66.5      | 97.0 | 23.2      |




# Quantitation Results Report (QT Reviewed)

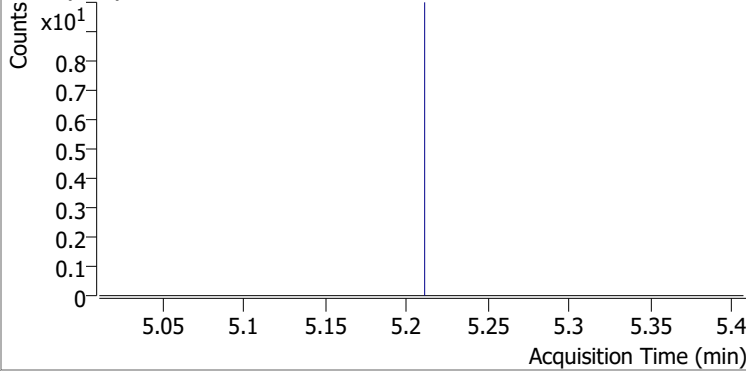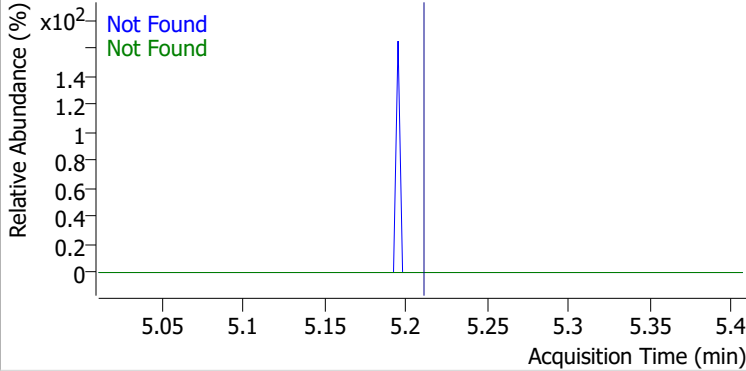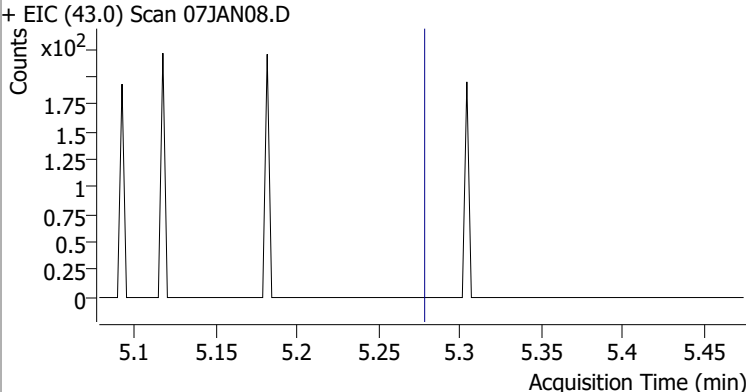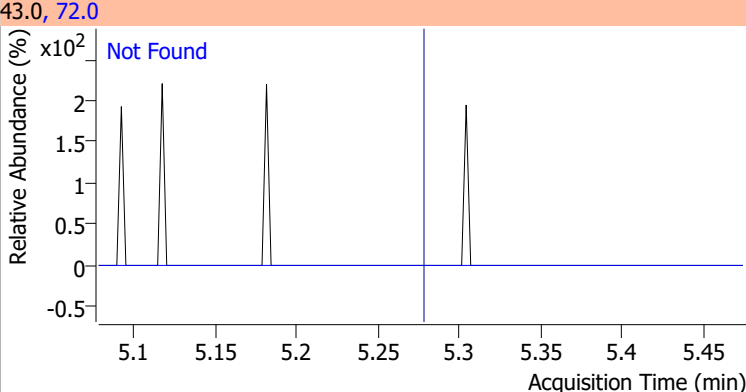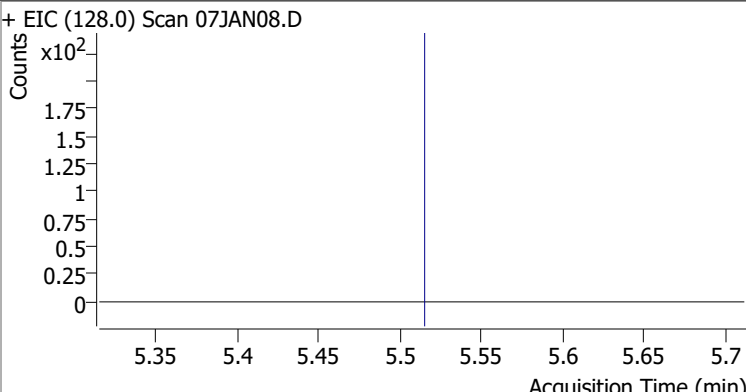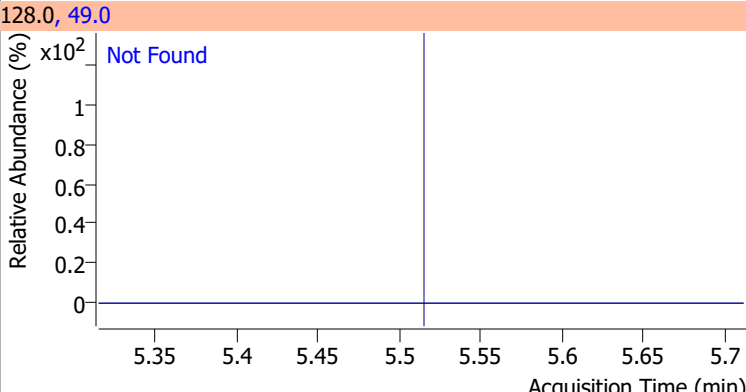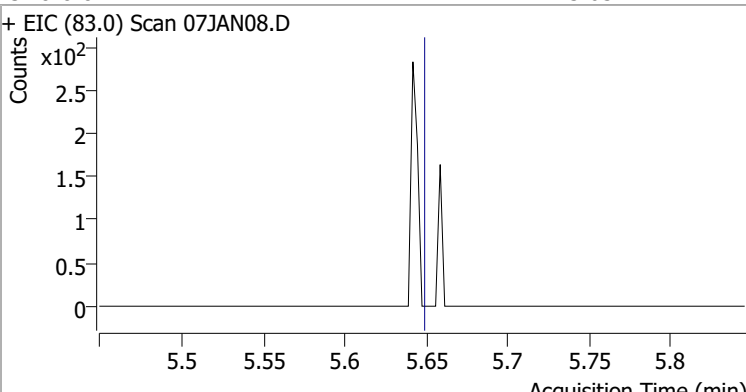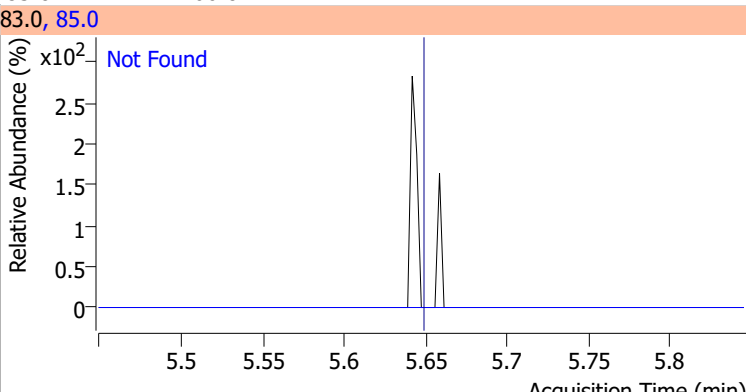
| Compound                                                                           | Conc. | Exp RT | QIon                                                                                 | Exp Ratio | QIon | Exp Ratio |
|------------------------------------------------------------------------------------|-------|--------|--------------------------------------------------------------------------------------|-----------|------|-----------|
| cis-1,2-Dichloroethene                                                             | N.D.  | 5.22   | 61.0                                                                                 | 167.2     | 98.0 | 67.3      |
| + EIC (96.0) Scan 07JAN08.D                                                        |       |        | 96.0, 61.0, 98.0                                                                     |           |      |           |
|    |       |        |    |           |      |           |
| Methyl ethyl ketone                                                                | N.D.  | 5.28   | 72.0                                                                                 | 21.3      |      |           |
| + EIC (43.0) Scan 07JAN08.D                                                        |       |        | 43.0, 72.0                                                                           |           |      |           |
|   |       |        |   |           |      |           |
| Bromochloromethane                                                                 | N.D.  | 5.52   | 49.0                                                                                 | 182.9     |      |           |
| + EIC (128.0) Scan 07JAN08.D                                                       |       |        | 128.0, 49.0                                                                          |           |      |           |
|  |       |        |  |           |      |           |
| Chloroform                                                                         | N.D.  | 5.65   | 85.0                                                                                 | 66.0      |      |           |
| + EIC (83.0) Scan 07JAN08.D                                                        |       |        | 83.0, 85.0                                                                           |           |      |           |
|  |       |        |  |           |      |           |

# Quantitation Results Report (QT Reviewed)


| Compound              | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------------|-------|--------|------|-----------|------|-----------|
| 1,1,1-Trichloroethane | N.D.  | 5.83   | 99.0 | 64.7      | 61.0 | 48.1      |




| Compound             | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Dibromofluoromethane | 275.6761 | 5.85 | 0.00     | 212882 | 191.5 | 22.1   | 0.0   | 53.1  |



| Compound             | Conc. | Exp RT | QIon  | Exp Ratio | QIon  | Exp Ratio |
|----------------------|-------|--------|-------|-----------|-------|-----------|
| Carbon tetrachloride | N.D.  | 6.02   | 119.0 | 97.2      | 121.0 | 30.1      |

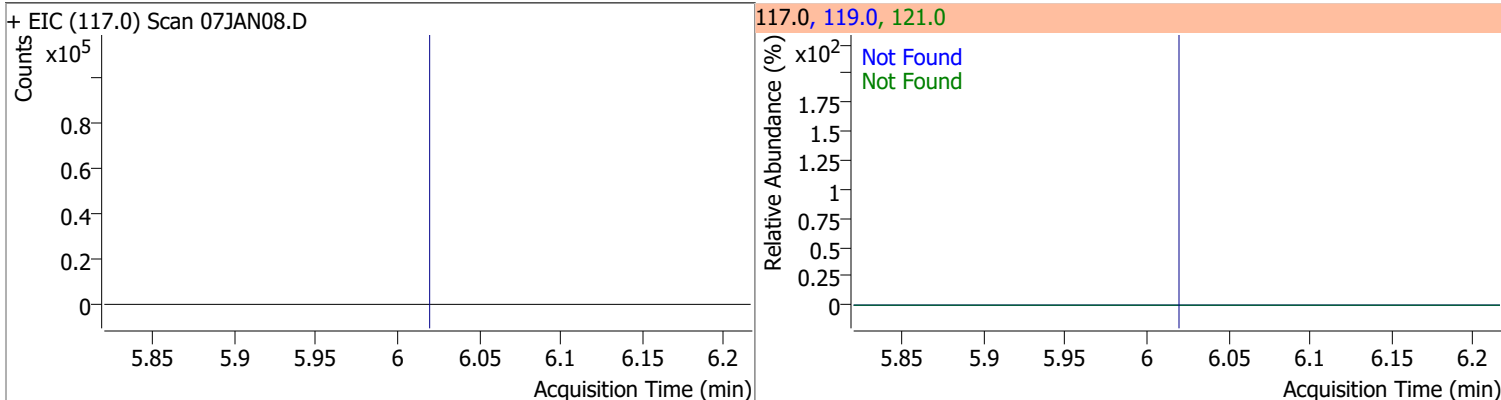


| Compound            | Conc. | Exp RT | QIon  | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|-------|-----------|------|-----------|
| 1,1-Dichloropropene | N.D.  | 6.04   | 110.0 | 35.9      | 77.0 | 30.1      |

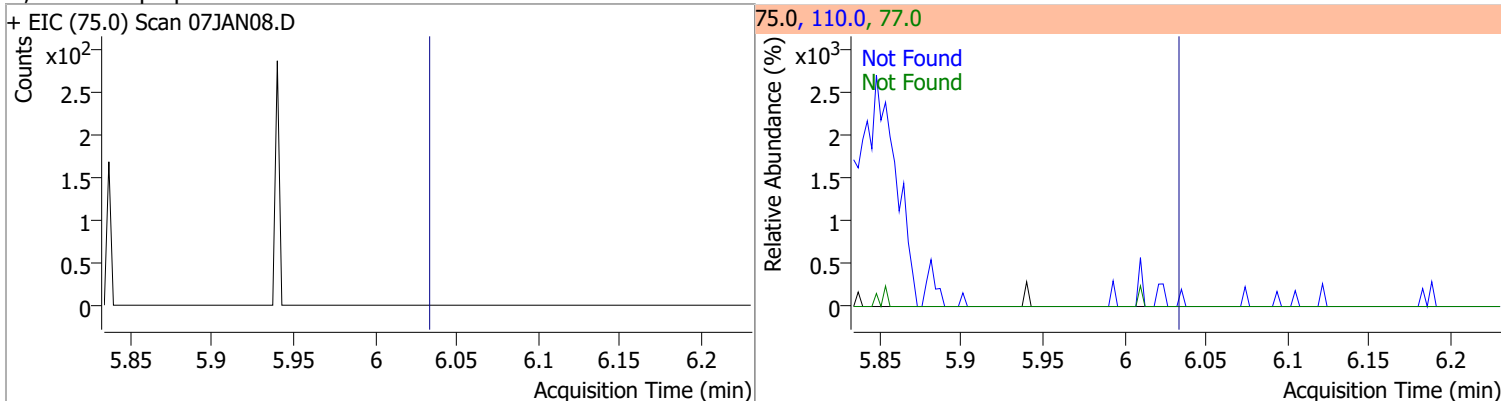


# Quantitation Results Report (QT Reviewed)


| Compound              | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 289.5314 | 6.23 | 0.00     | 96571 | 65.0 | 192.1  | 166.5 | 226.5 |




| Compound | Conc.  | RT   | Dev(Min) | Resp.   | QIon | QRatio | Lower | Upper |
|----------|--------|------|----------|---------|------|--------|-------|-------|
| Benzene  | 0.0648 | 6.27 | 0.00     | 212 (m) | 77.0 | 39.9   | 0.0   | 53.5  |











| Compound           | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,2-Dichloroethane | N.D.  | 6.32   | 64.0 | 29.9      | 98.0 | 7.6       |



| Compound        | Conc. | Exp RT | QIon  | Exp Ratio | QIon | Exp Ratio |
|-----------------|-------|--------|-------|-----------|------|-----------|
| Trichloroethene | N.D.  | 7.03   | 130.0 | 101.5     | 97.0 | 64.1      |




# Quantitation Results Report (QT Reviewed)

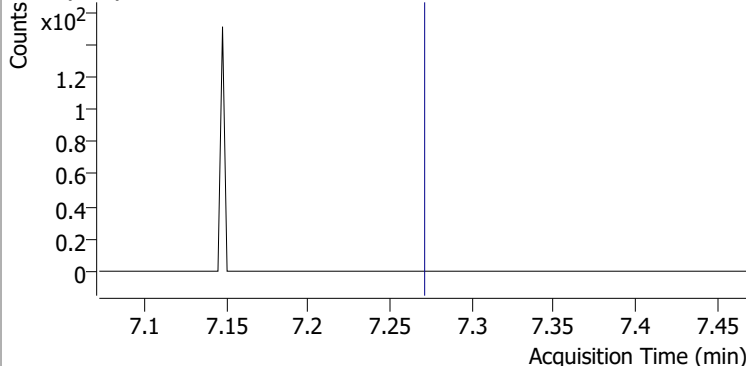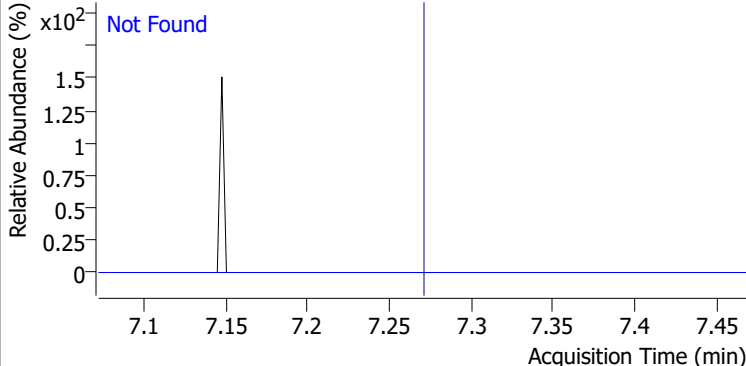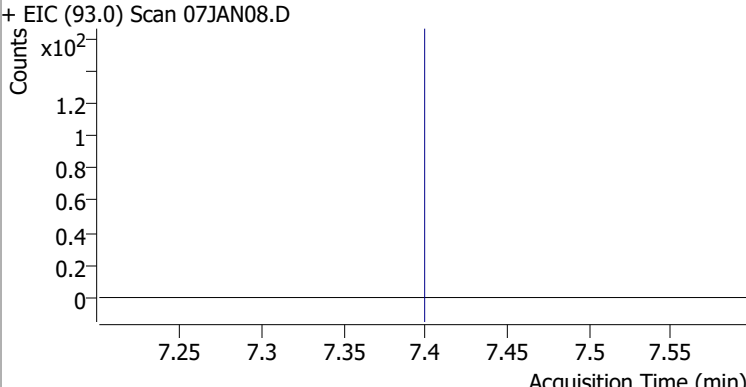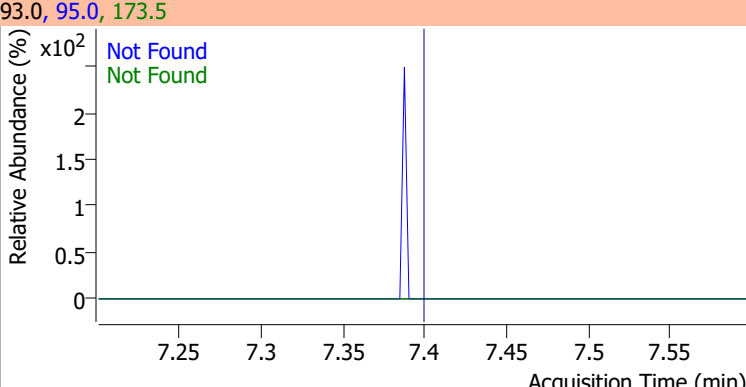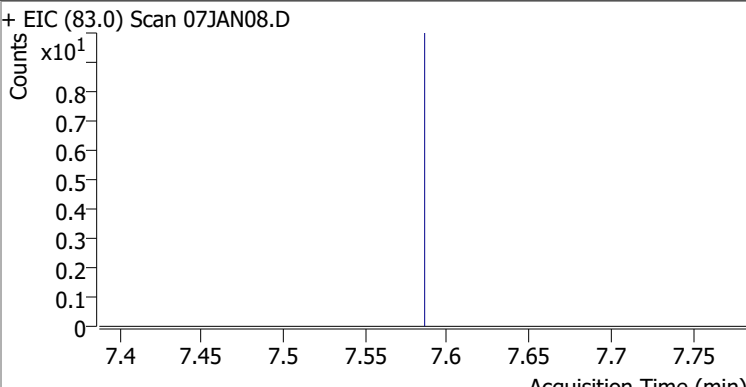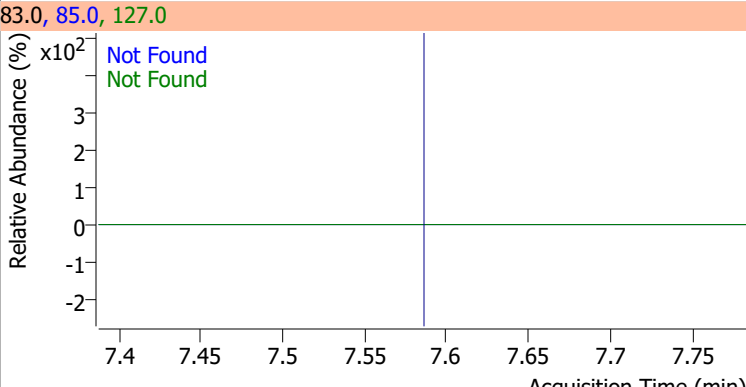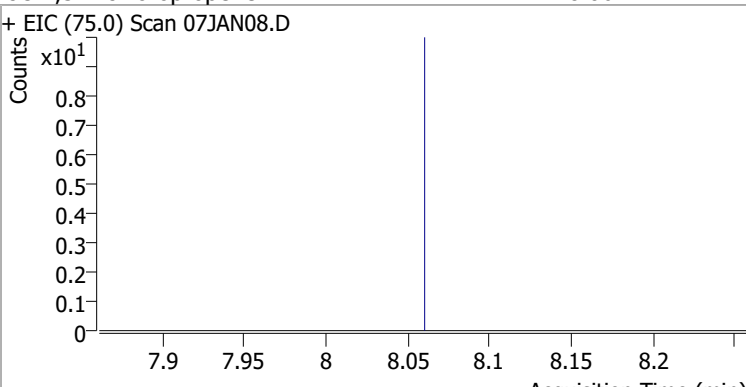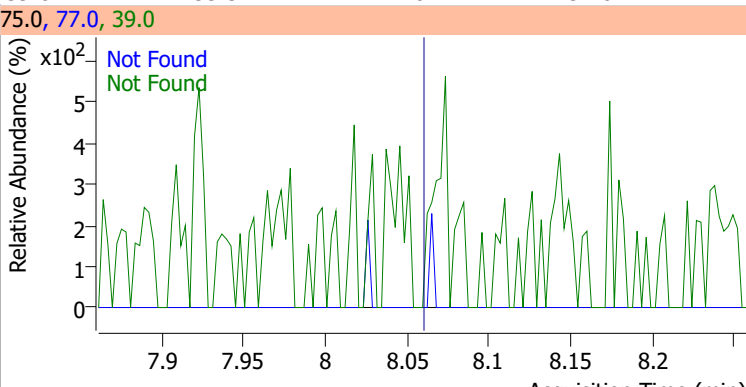
| Compound                                                                           | Conc. | Exp RT | QIon                                                                                 | Exp Ratio |      |           |
|------------------------------------------------------------------------------------|-------|--------|--------------------------------------------------------------------------------------|-----------|------|-----------|
| 1,2-Dichloropropane                                                                | N.D.  | 7.27   | 76.0                                                                                 | 38.2      |      |           |
| + EIC (63.0) Scan 07JAN08.D                                                        |       |        | 63.0, 76.0                                                                           |           |      |           |
|    |       |        |    |           |      |           |
| Dibromomethane                                                                     | N.D.  | 7.40   | 173.5                                                                                | 113.7     | QIon | Exp Ratio |
| + EIC (93.0) Scan 07JAN08.D                                                        |       |        | 93.0, 95.0, 173.5                                                                    |           |      |           |
|   |       |        |   |           |      |           |
| Bromodichloromethane                                                               | N.D.  | 7.59   | 85.0                                                                                 | 64.5      | QIon | Exp Ratio |
| + EIC (83.0) Scan 07JAN08.D                                                        |       |        | 83.0, 85.0, 127.0                                                                    |           |      |           |
|  |       |        |  |           |      |           |
| cis-1,3-Dichloropropene                                                            | N.D.  | 8.06   | 39.0                                                                                 | 53.3      | QIon | Exp Ratio |
| + EIC (75.0) Scan 07JAN08.D                                                        |       |        | 75.0, 77.0, 39.0                                                                     |           |      |           |
|  |       |        |  |           |      |           |

# Quantitation Results Report (QT Reviewed)


| Compound   | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 263.8953 | 8.32 | 0.00     | 818871 | 100.0 | 63.9   | 34.4  | 94.4  |
|            |          |      |          |        | 99.0  | 9.4    | 0.0   | 39.6  |

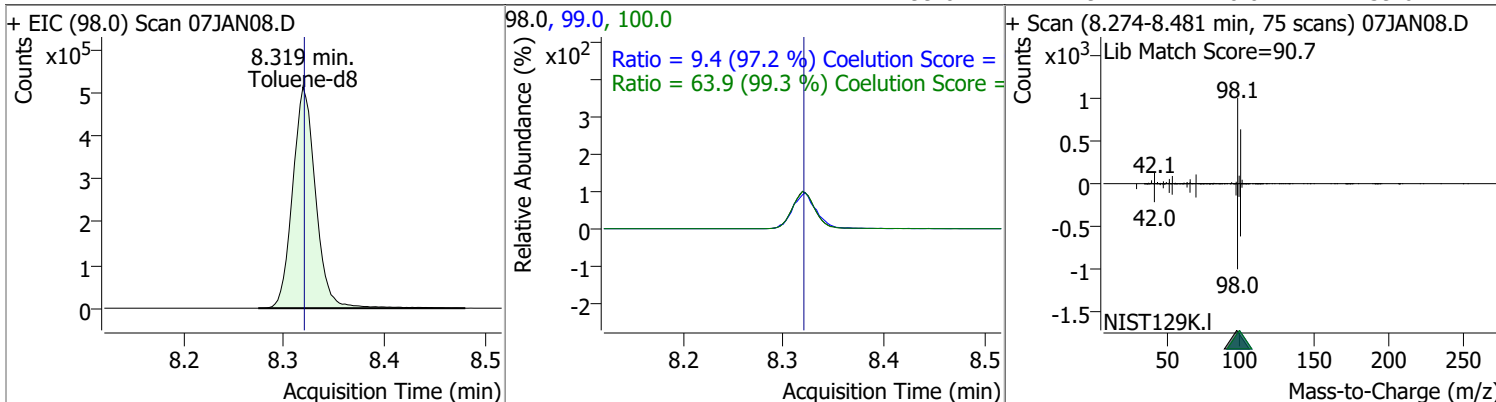


| Compound | Conc.  | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|--------|------|----------|-------|------|--------|-------|-------|
| Toluene  | 1.8091 | 8.39 | 0.00     | 3792  | 91.0 | 182.3  | 145.8 | 205.8 |

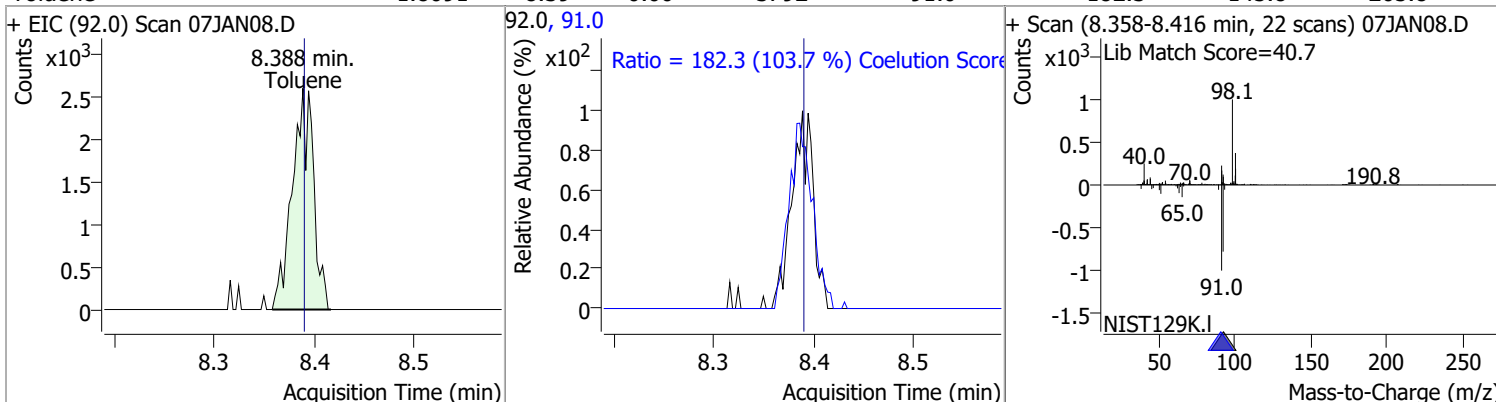

| Compound                  | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,3-Dichloropropene | N.D.  | 8.64   | 39.0 | 53.4      | 77.0 | 32.4      |

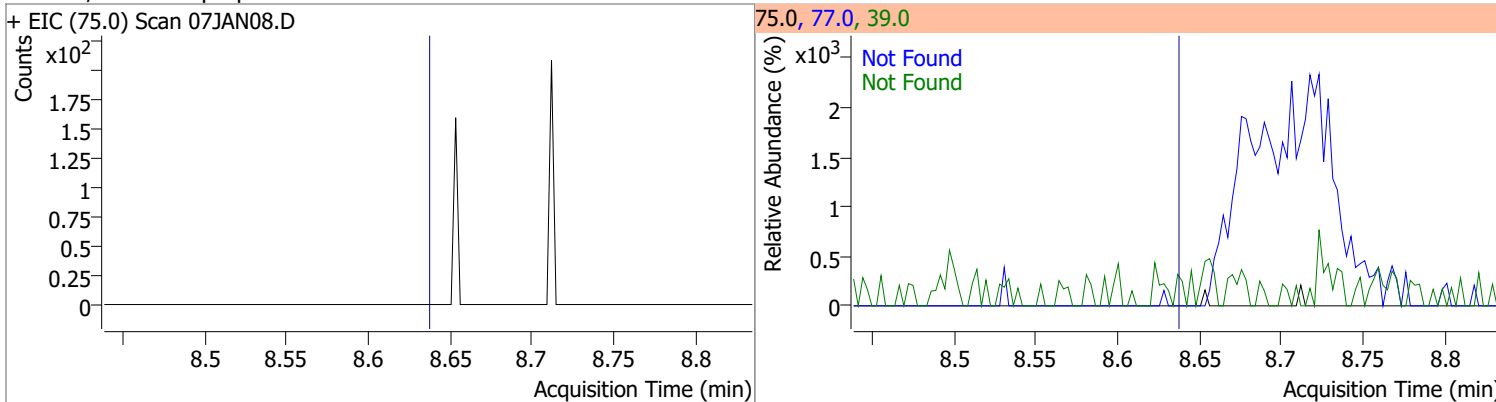


| Compound              | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------------|-------|--------|------|-----------|------|-----------|
| 1,1,2-Trichloroethane | N.D.  | 8.82   | 97.0 | 114.6     | 85.0 | 67.6      |

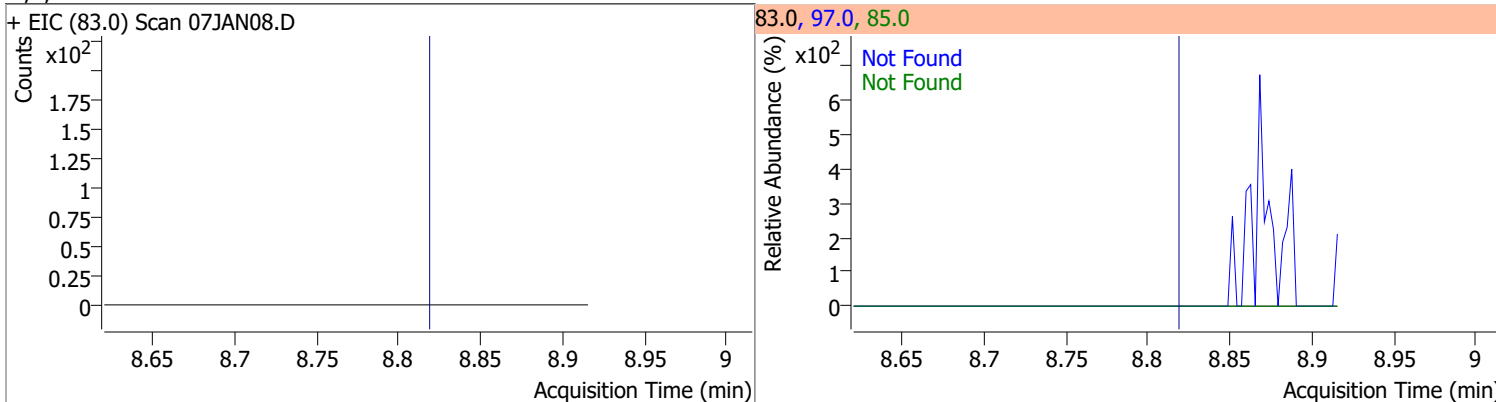




# Quantitation Results Report (QT Reviewed)


| Compound          | Conc. | Exp RT | QIon  | Exp Ratio | QIon  | Exp Ratio |
|-------------------|-------|--------|-------|-----------|-------|-----------|
| Tetrachloroethene | N.D.  | 8.94   | 165.8 | 128.6     | 129.0 | 91.5      |

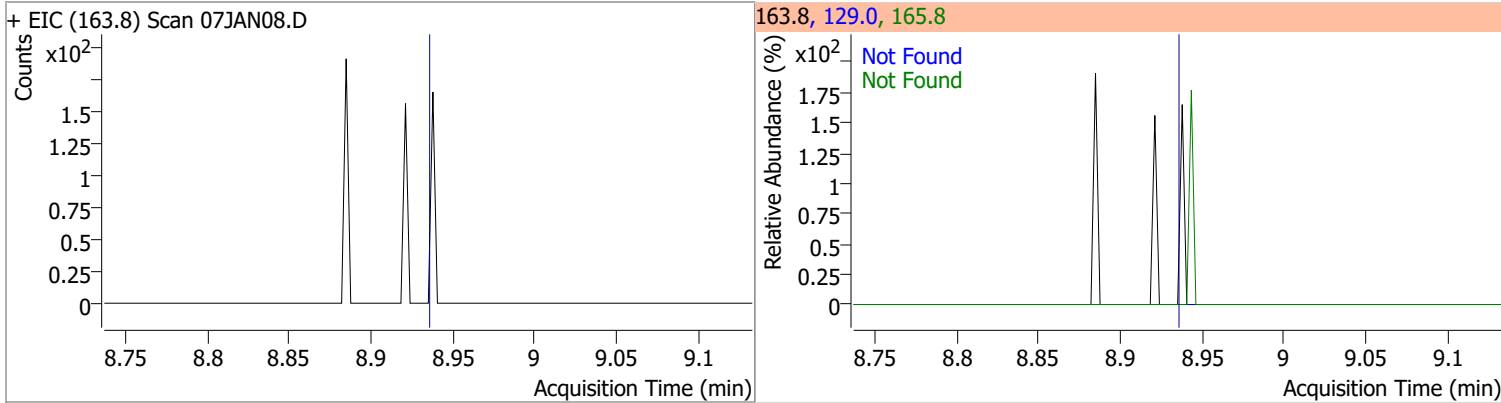


| Compound            | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| 1,3-Dichloropropane | N.D.  | 8.98   | 78.0 | 32.9      |







| Compound             | Conc. | Exp RT | QIon  | Exp Ratio |
|----------------------|-------|--------|-------|-----------|
| Chlorodibromomethane | N.D.  | 9.21   | 127.0 | 78.0      |

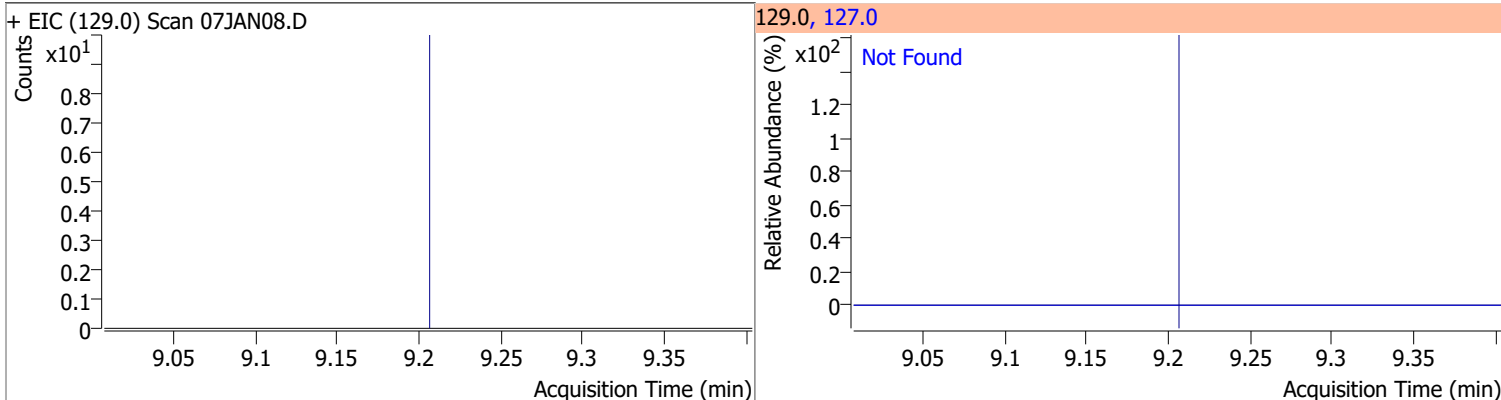

| Compound          | Conc. | Exp RT | QIon  | Exp Ratio |
|-------------------|-------|--------|-------|-----------|
| 1,2-Dibromoethane | N.D.  | 9.31   | 109.0 | 94.5      |

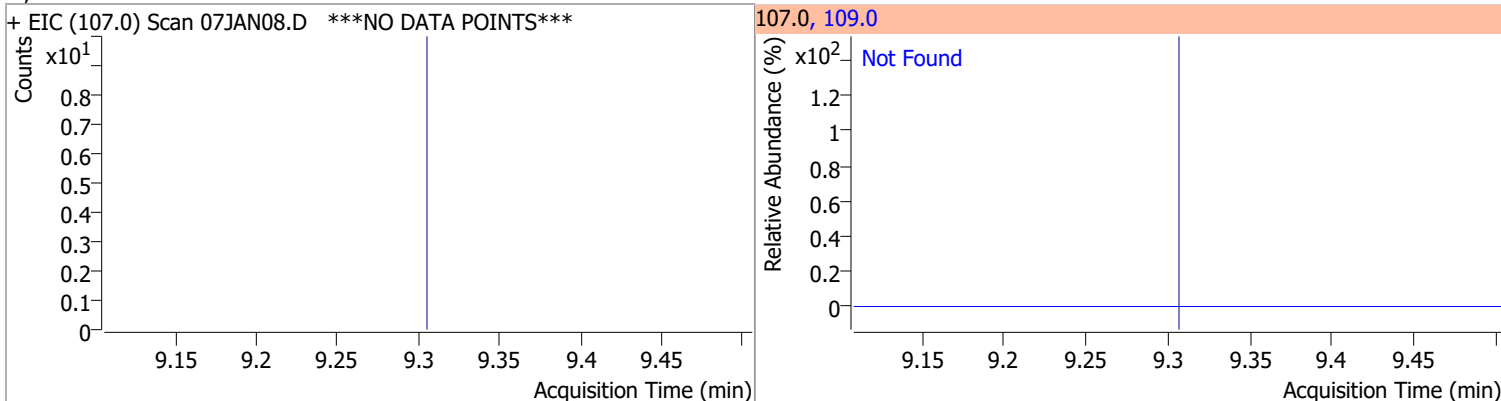


# Quantitation Results Report (QT Reviewed)

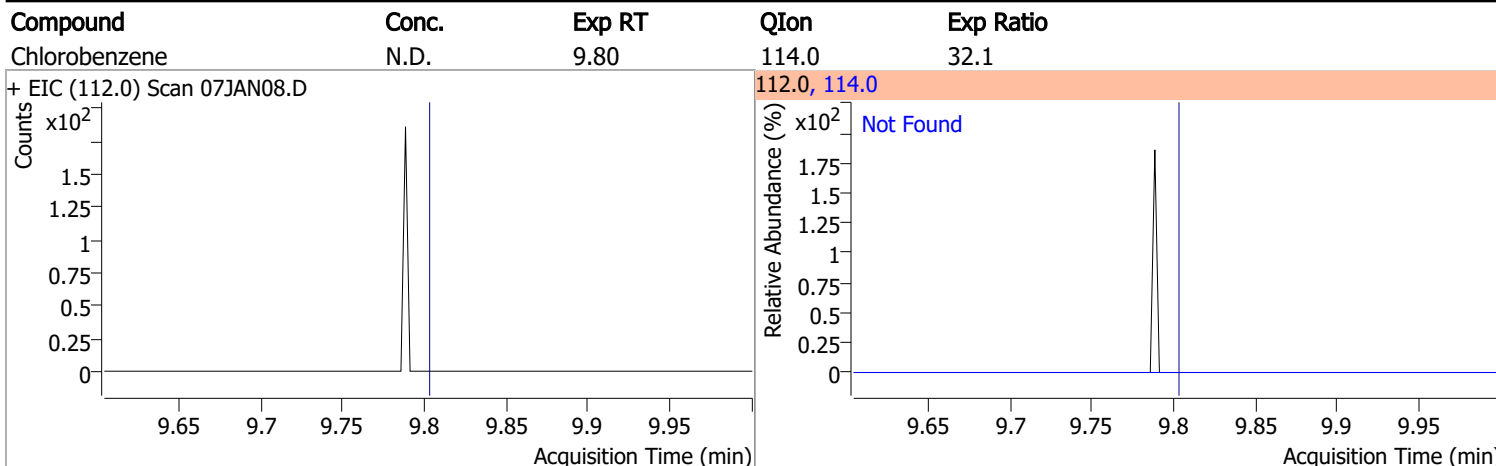


# Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------|-------|--------|------|-----------|
| o-Xylene | N.D.  | 10.43  | 91.0 | 213.1     |




| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------|-------|--------|------|-----------|
| Styrene  | N.D.  | 10.45  | 78.0 | 49.6      |











| Compound  | Conc. | Exp RT | QIon  | Exp Ratio | QIon  | Exp Ratio |
|-----------|-------|--------|-------|-----------|-------|-----------|
| Bromoform | N.D.  | 10.63  | 170.5 | 52.1      | 174.5 | 50.1      |











| Compound             | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 279.2702 | 10.95 | 0.00     | 240793 | 174.0 | 93.1   | 61.7  | 121.7 |
|                      |          |       |          |        | 176.0 | 89.6   | 60.6  | 120.6 |



# Quantitation Results Report (QT Reviewed)

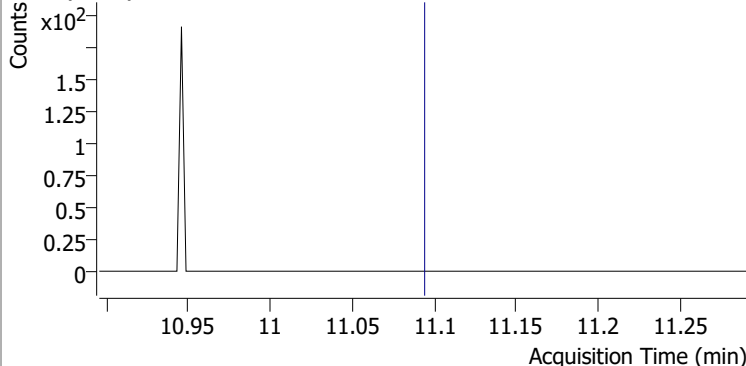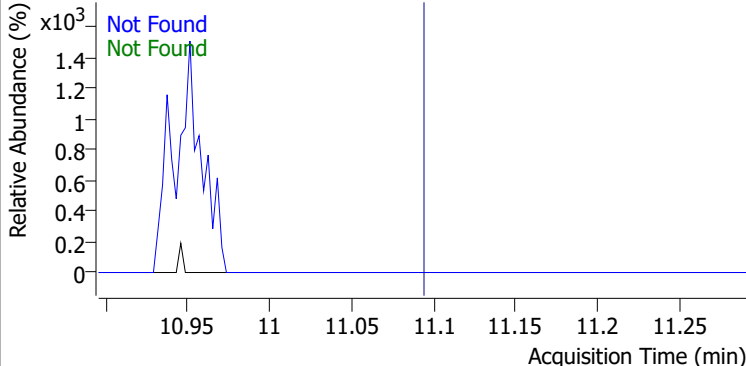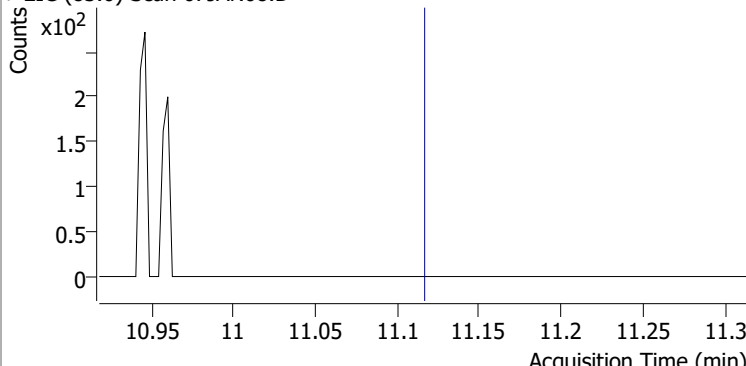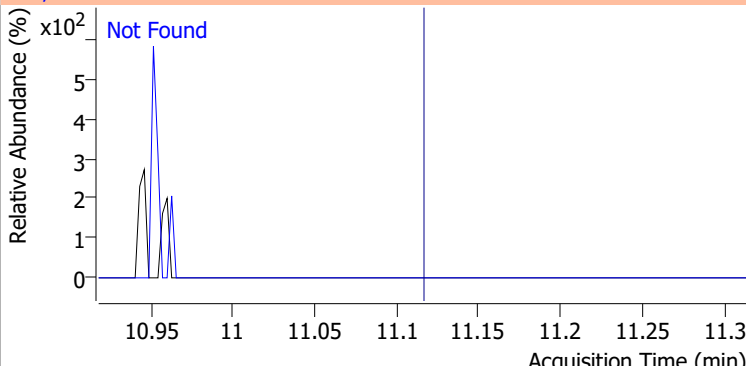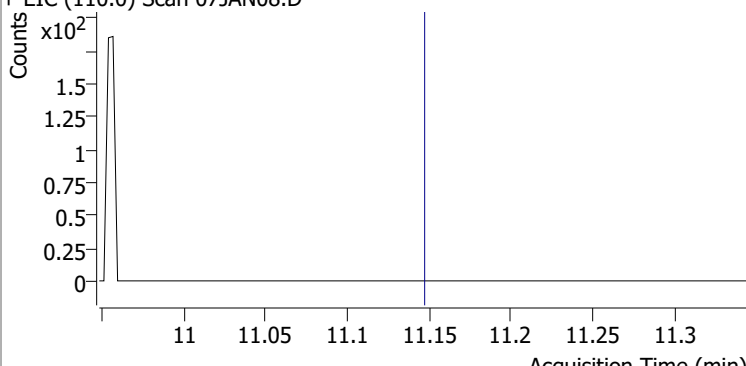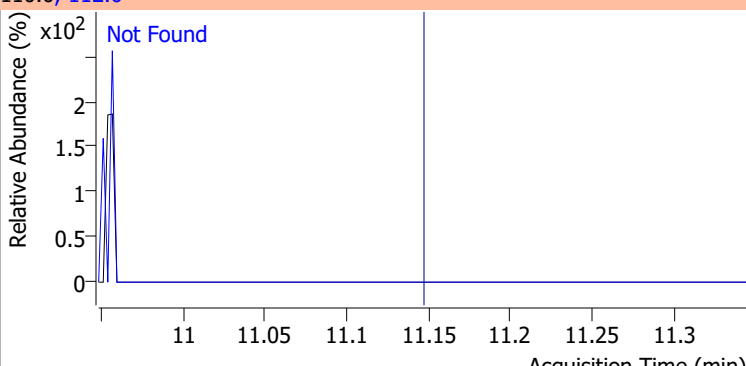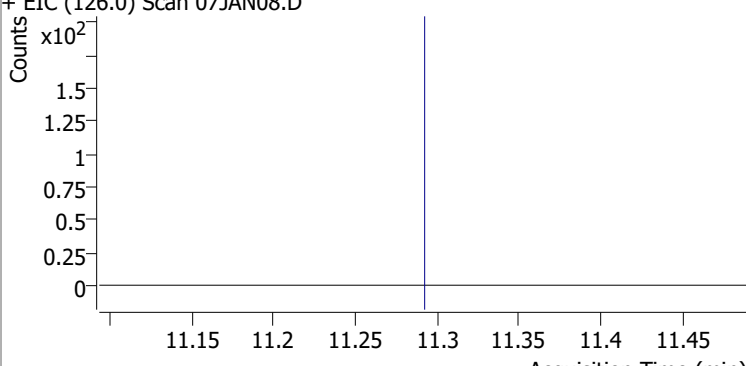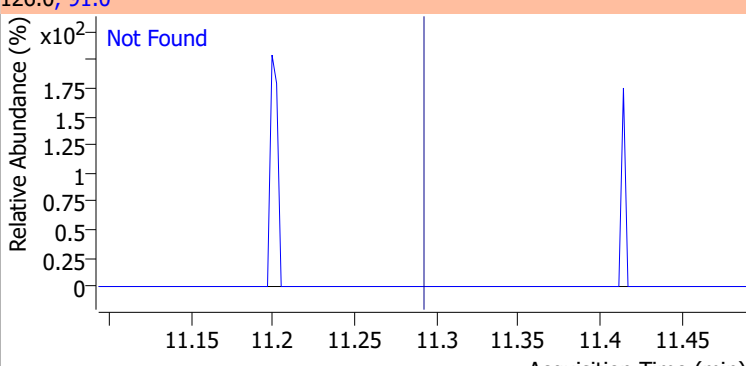
| Compound                                                                           | Conc. | Exp RT | QIon                                                                                 | Exp Ratio | QIon  | Exp Ratio |
|------------------------------------------------------------------------------------|-------|--------|--------------------------------------------------------------------------------------|-----------|-------|-----------|
| Bromobenzene                                                                       | N.D.  | 11.09  | 77.0                                                                                 | 145.7     | 158.0 | 96.5      |
| + EIC (156.0) Scan 07JAN08.D                                                       |       |        | 156.0, 77.0, 158.0                                                                   |           |       |           |
|    |       |        |    |           |       |           |
| 1,1,2,2-Tetrachloroethane                                                          | N.D.  | 11.12  | 85.0                                                                                 | 66.2      |       |           |
| + EIC (83.0) Scan 07JAN08.D                                                        |       |        | 83.0, 85.0                                                                           |           |       |           |
|   |       |        |   |           |       |           |
| 1,2,3-Trichloropropane                                                             | N.D.  | 11.15  | 112.0                                                                                | 63.5      |       |           |
| + EIC (110.0) Scan 07JAN08.D                                                       |       |        | 110.0, 112.0                                                                         |           |       |           |
|  |       |        |  |           |       |           |
| 2-Chlorotoluene                                                                    | N.D.  | 11.29  | 91.0                                                                                 | 282.3     |       |           |
| + EIC (126.0) Scan 07JAN08.D                                                       |       |        | 126.0, 91.0                                                                          |           |       |           |
|  |       |        |  |           |       |           |

# Quantitation Results Report (QT Reviewed)
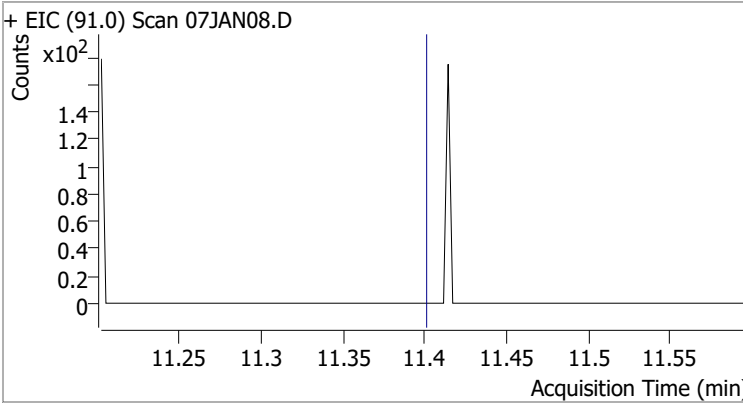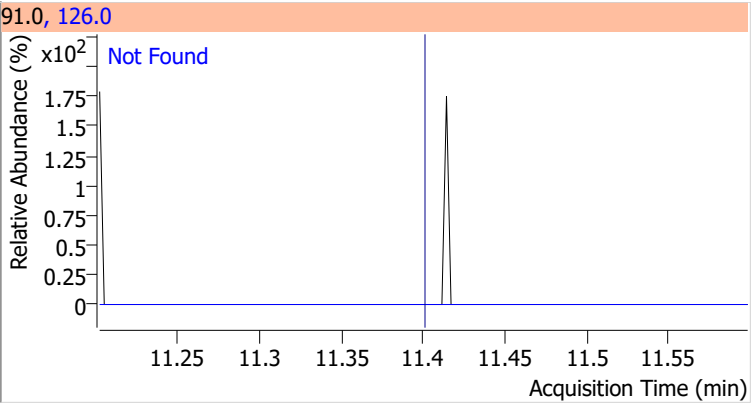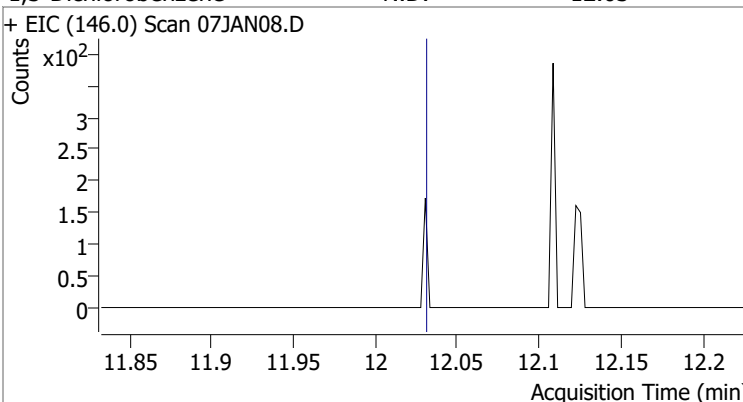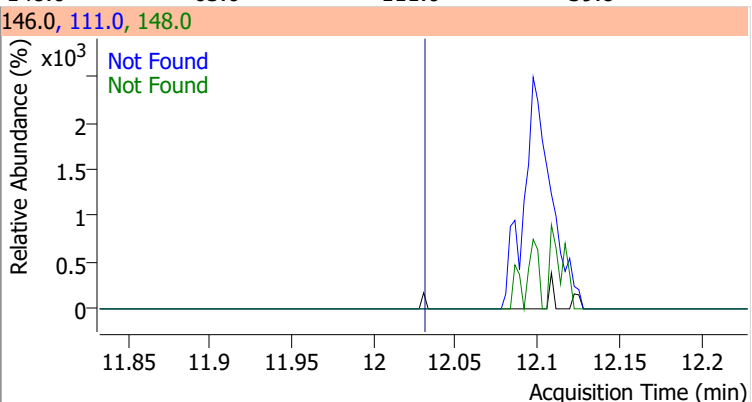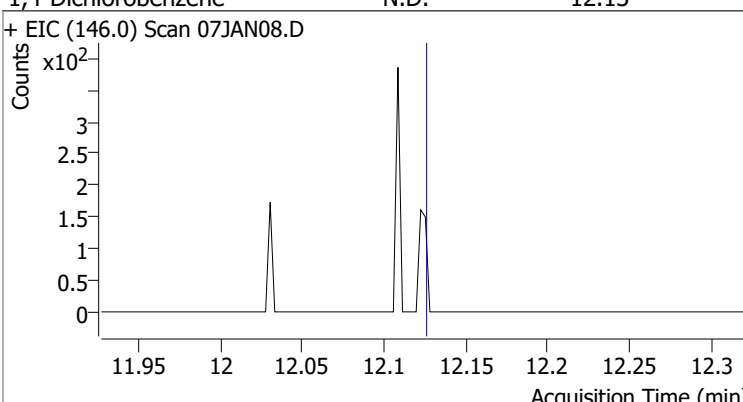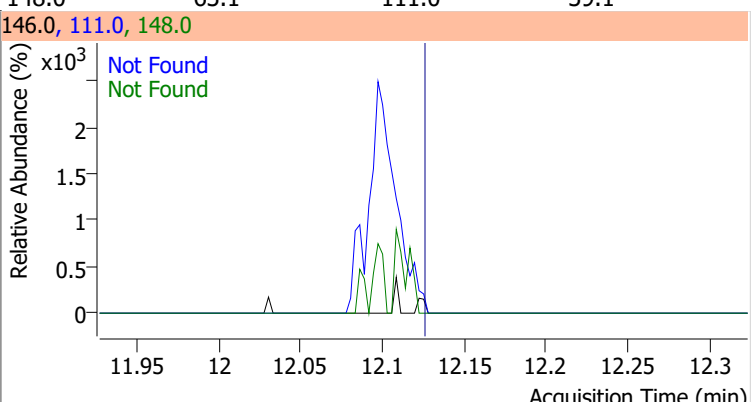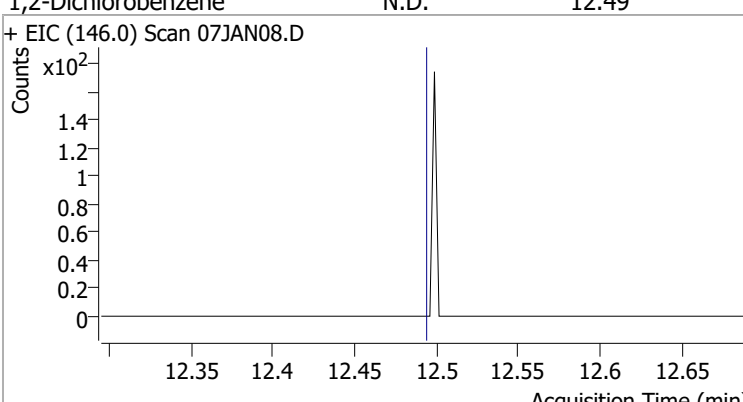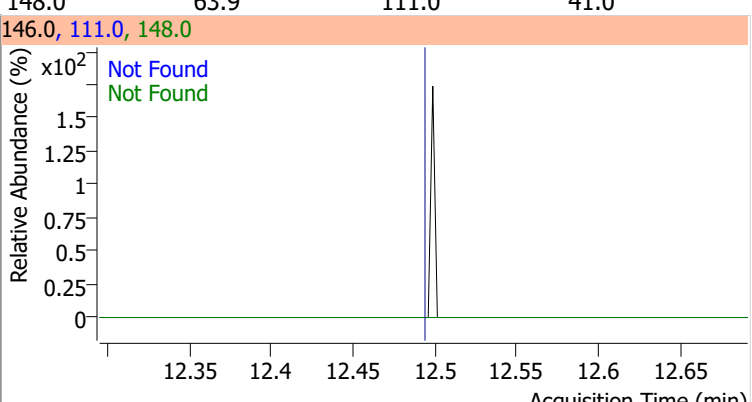
| Compound                                                                           | Conc. | Exp RT | QIon                                                                                 | Exp Ratio |      |           |
|------------------------------------------------------------------------------------|-------|--------|--------------------------------------------------------------------------------------|-----------|------|-----------|
| 4-Chlorotoluene                                                                    | N.D.  | 11.40  | 126.0                                                                                | 31.7      |      |           |
| + EIC (91.0) Scan 07JAN08.D                                                        |       |        | 91.0, 126.0                                                                          |           |      |           |
|    |       |        |    |           |      |           |
| 1,3-Dichlorobenzene                                                                | N.D.  | 12.03  | 148.0                                                                                | 63.6      | QIon | Exp Ratio |
| + EIC (146.0) Scan 07JAN08.D                                                       |       |        | 146.0, 111.0, 148.0                                                                  |           |      |           |
|    |       |        |    |           |      |           |
| 1,4-Dichlorobenzene                                                                | N.D.  | 12.13  | 148.0                                                                                | 63.1      | QIon | Exp Ratio |
| + EIC (146.0) Scan 07JAN08.D                                                       |       |        | 146.0, 111.0, 148.0                                                                  |           |      |           |
|  |       |        |  |           |      |           |
| 1,2-Dichlorobenzene                                                                | N.D.  | 12.49  | 148.0                                                                                | 63.9      | QIon | Exp Ratio |
| + EIC (146.0) Scan 07JAN08.D                                                       |       |        | 146.0, 111.0, 148.0                                                                  |           |      |           |
|  |       |        |  |           |      |           |

# Quantitation Results Report (QT Reviewed)

|                |                                     |                   |                       |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File      | 07JAN09.D                           | Operator          | MSC                   |
| Acq. Method    | 5975CACQF.M                         | Acq. Date-Time    | 1/7/2022 1:19:35 PM   |
| Sample Name    | B22010262-002A                      | Instrument        | VOA5975C              |
| Vial           | 9                                   | Multiplier        | 1.00                  |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m  | Comment           |                       |
| Tune File      | BFB_Atune3.u                        | Tune Date         | 10/11/2021 4:02:00 PM |
| Batch Name     | VG010722_8260B.batch.bin            | Last Calib Update | 3/2/2022 10:41:44 AM  |
| Ref Library    | \\MASSHUNTER\Org\Library\NIST129K.I |                   |                       |

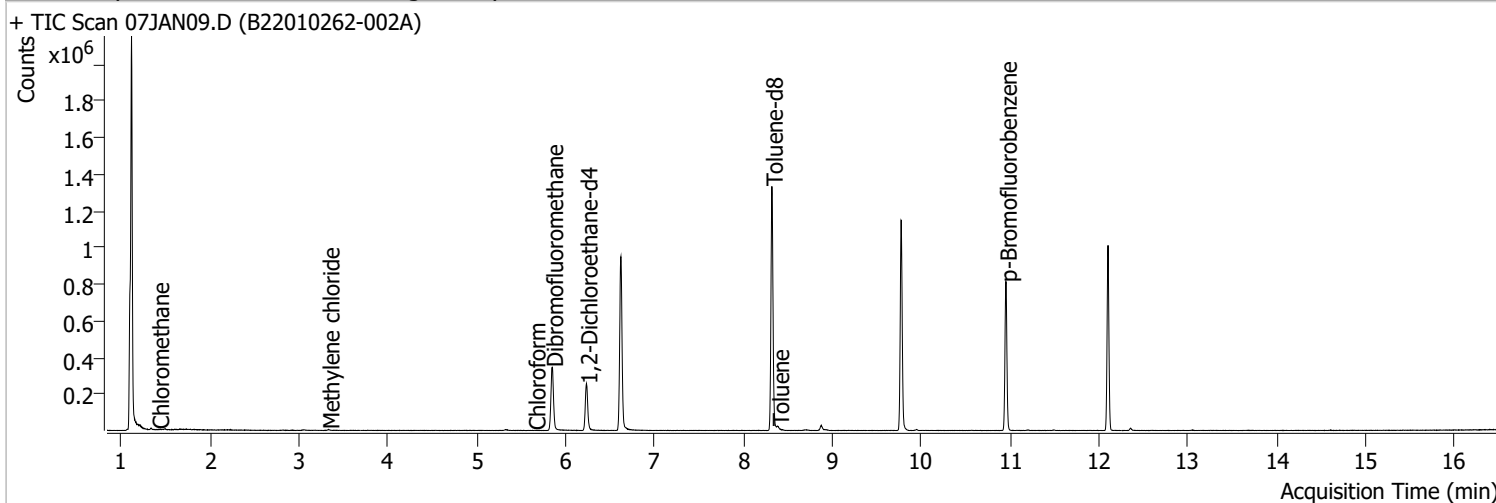





| Compound                           | RT                   | QIon  | Resp.  | Conc.              | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|--------------------|-------|----------|
| <b>Internal Standards</b>          |                      |       |        |                    |       |          |
| M Fluorobenzene                    | 6.621                | 96.0  | 811488 | 250.0000           | ng    | -0.003   |
| M Chlorobenzene-d5                 | 9.772                | 82.0  | 311589 | 250.0000           | ng    | 0.000    |
| M 1,4-Dichlorobenzene-d4           | 12.100               | 152.0 | 236584 | 250.0000           | ng    | 0.000    |
| <b>System Monitoring Compounds</b> |                      |       |        |                    |       |          |
| S Dibromofluoromethane             | 5.845                | 113.0 | 211827 | 277.0777           | ng    | 0.000    |
| Spiked Amount: 250.000             | Range: 80.0 - 119.0% |       |        | Recovery = 110.83% |       |          |
| S 1,2-Dichloroethane-d4            | 6.233                | 67.0  | 92974  | 281.5597           | ng    | 0.000    |
| Spiked Amount: 250.000             | Range: 81.0 - 118.0% |       |        | Recovery = 112.62% |       |          |
| S Toluene-d8                       | 8.319                | 98.0  | 816456 | 271.9136           | ng    | 0.000    |
| Spiked Amount: 250.000             | Range: 89.0 - 112.0% |       |        | Recovery = 108.77% |       |          |
| S p-Bromofluorobenzene             | 10.951               | 95.0  | 234685 | 270.7711           | ng    | -0.003   |
| Spiked Amount: 250.000             | Range: 85.0 - 114.0% |       |        | Recovery = 108.31% |       |          |
| <b>Target Compounds</b>            |                      |       |        |                    |       |          |
| T Dichlorodifluoromethane          | 0.000                |       | 0      | N.D.               |       |          |
| T Chloromethane                    | 1.414                | 50.0  | 1041   | 0.8064             | ng    | m 85     |
| T Vinyl chloride                   | 0.000                |       | 0      | N.D.               |       |          |
| T Bromomethane                     | 0.000                |       | 0      | N.D.               |       |          |
| T Chloroethane                     | 0.000                |       | 0      | N.D.               |       |          |
| T Trichlorofluoromethane           | 0.000                |       | 0      | N.D.               |       |          |
| T 1,1-Dichloroethene               | 0.000                |       | 0      | N.D.               |       |          |
| T Methylene chloride               | 3.330                | 49.0  | 2658   | 2.2061             | ng    | m 98     |
| T trans-1,2-Dichloroethene         | 0.000                |       | 0      | N.D.               |       |          |
| T Methyl tert-butyl ether (MTBE)   | 0.000                |       | 0      | N.D.               |       |          |
| T 1,1-Dichloroethane               | 0.000                |       | 0      | N.D.               |       |          |
| T 2,2-Dichloropropane              | 0.000                |       | 0      | N.D.               |       |          |
| T cis-1,2-Dichloroethene           | 0.000                |       | 0      | N.D.               |       |          |
| T Methyl ethyl ketone              | 0.000                |       | 0      | N.D.               |       |          |
| T Bromochloromethane               | 0.000                |       | 0      | N.D.               |       |          |
| T Chloroform                       | 5.650                | 83.0  | 381    | 0.2466             | ng    | m 99     |

# Quantitation Results Report (QT Reviewed)

| Compound                    | RT    | QIon | Resp. | Conc.  | Units | Dev(Min) |
|-----------------------------|-------|------|-------|--------|-------|----------|
| T 1,1,1-Trichloroethane     | 0.000 |      | 0     | N.D.   |       |          |
| T Carbon tetrachloride      | 0.000 |      | 0     | N.D.   |       |          |
| T 1,1-Dichloropropene       | 0.000 |      | 0     | N.D.   |       |          |
| T Benzene                   | 0.000 |      | 0     | N.D.   |       |          |
| T 1,2-Dichloroethane        | 0.000 |      | 0     | N.D.   |       |          |
| T Trichloroethene           | 0.000 |      | 0     | N.D.   |       |          |
| T 1,2-Dichloropropane       | 0.000 |      | 0     | N.D.   |       |          |
| T Dibromomethane            | 0.000 |      | 0     | N.D.   |       |          |
| T Bromodichloromethane      | 0.000 |      | 0     | N.D.   |       |          |
| T cis-1,3-Dichloropropene   | 0.000 |      | 0     | N.D.   |       |          |
| T Toluene                   | 8.391 | 92.0 | 4452  | 2.1950 | ng    | 99       |
| T trans-1,3-Dichloropropene | 0.000 |      | 0     | N.D.   |       |          |
| T 1,1,2-Trichloroethane     | 0.000 |      | 0     | N.D.   |       |          |
| T Tetrachloroethene         | 0.000 |      | 0     | N.D.   |       |          |
| T 1,3-Dichloropropane       | 0.000 |      | 0     | N.D.   |       |          |
| T Chlorodibromomethane      | 0.000 |      | 0     | N.D.   |       |          |
| T 1,2-Dibromoethane         | 0.000 |      | 0     | N.D.   |       |          |
| T Chlorobenzene             | 0.000 |      | 0     | N.D.   |       |          |
| T 1,1,1,2-Tetrachloroethane | 0.000 |      | 0     | N.D.   |       |          |
| T Ethylbenzene              | 0.000 |      | 0     | N.D.   |       |          |
| T m+p-Xylenes               | 0.000 |      | 0     | N.D.   |       |          |
| T o-Xylene                  | 0.000 |      | 0     | N.D.   |       |          |
| T Styrene                   | 0.000 |      | 0     | N.D.   |       |          |
| T Bromoform                 | 0.000 |      | 0     | N.D.   |       |          |
| T Bromobenzene              | 0.000 |      | 0     | N.D.   |       |          |
| T 1,1,2,2-Tetrachloroethane | 0.000 |      | 0     | N.D.   |       |          |
| T 1,2,3-Trichloropropane    | 0.000 |      | 0     | N.D.   |       |          |
| T 2-Chlorotoluene           | 0.000 |      | 0     | N.D.   |       |          |
| T 4-Chlorotoluene           | 0.000 |      | 0     | N.D.   |       |          |
| T 1,3-Dichlorobenzene       | 0.000 |      | 0     | N.D.   |       |          |
| T 1,4-Dichlorobenzene       | 0.000 |      | 0     | N.D.   |       |          |
| T 1,2-Dichlorobenzene       | 0.000 |      | 0     | N.D.   |       |          |

(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (\*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak


# Quantitation Results Report (QT Reviewed)

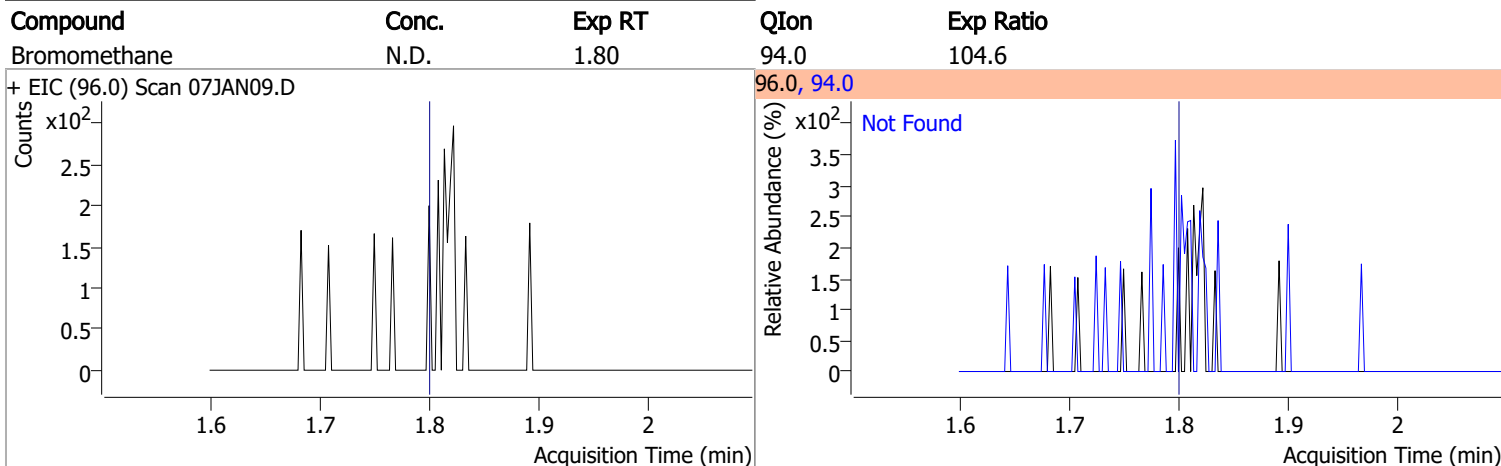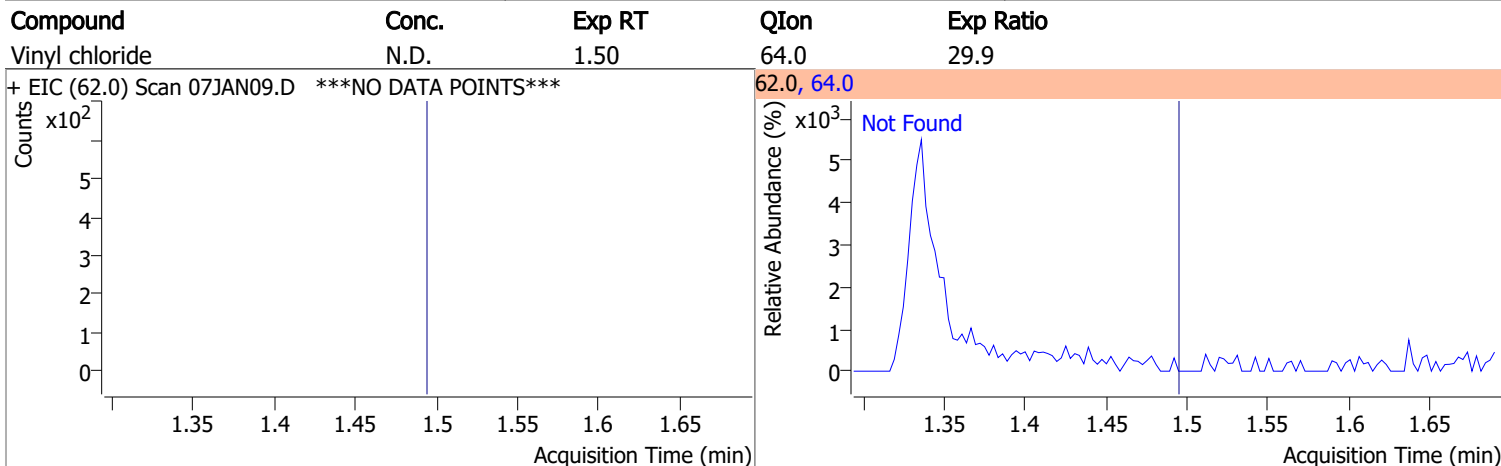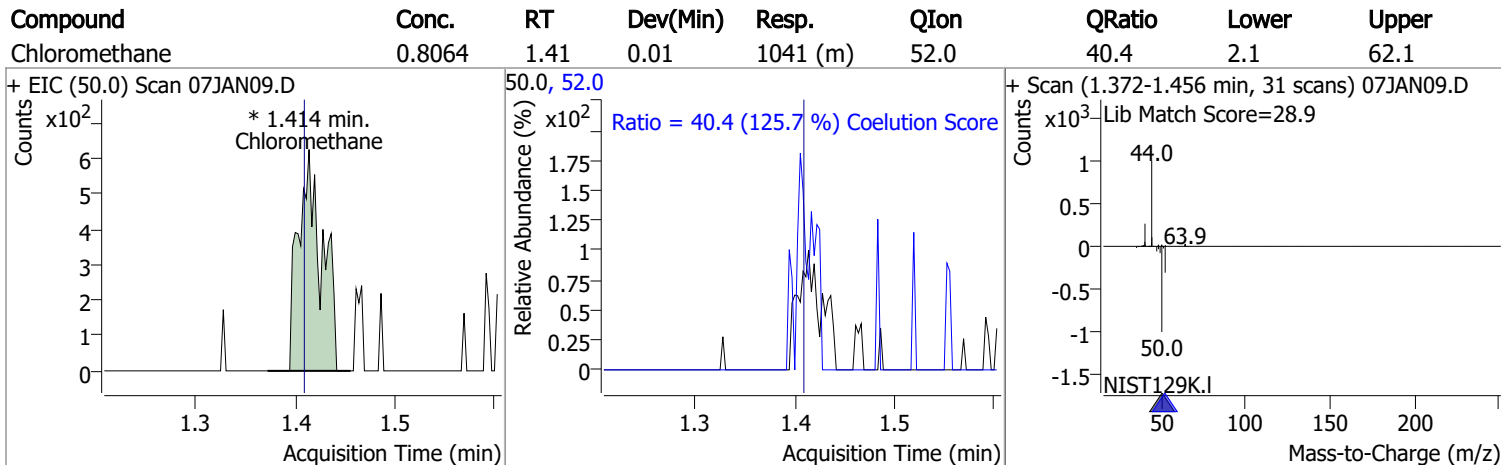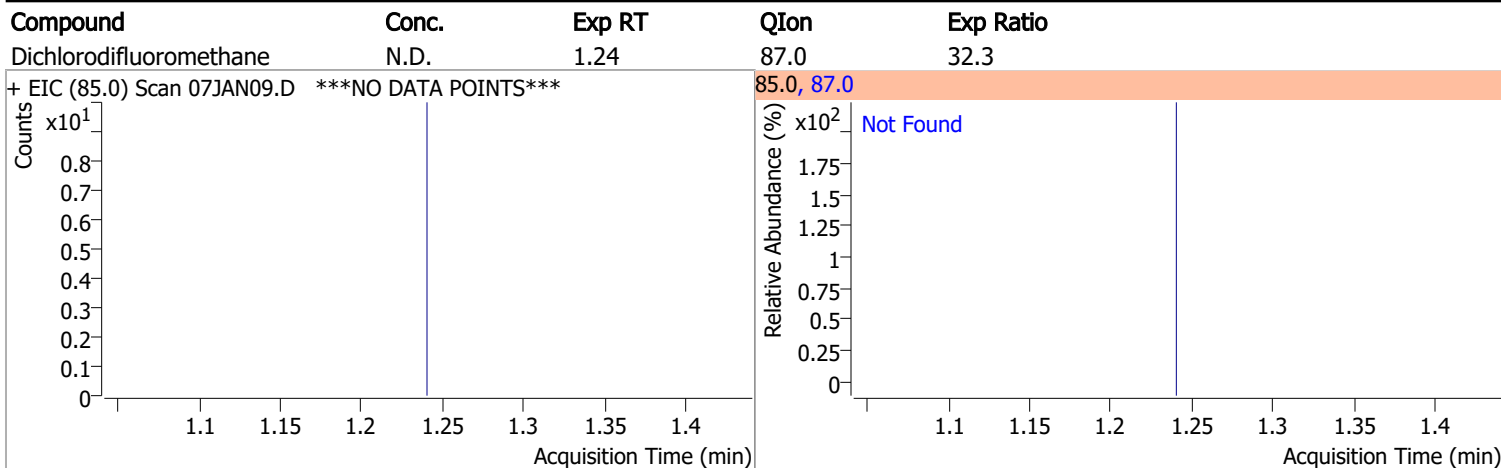




# Quantitation Results Report (QT Reviewed)


| Compound     | Conc. | Exp RT | QIon | Exp Ratio |
|--------------|-------|--------|------|-----------|
| Chloroethane | N.D.  | 1.89   | 66.0 | 30.1      |

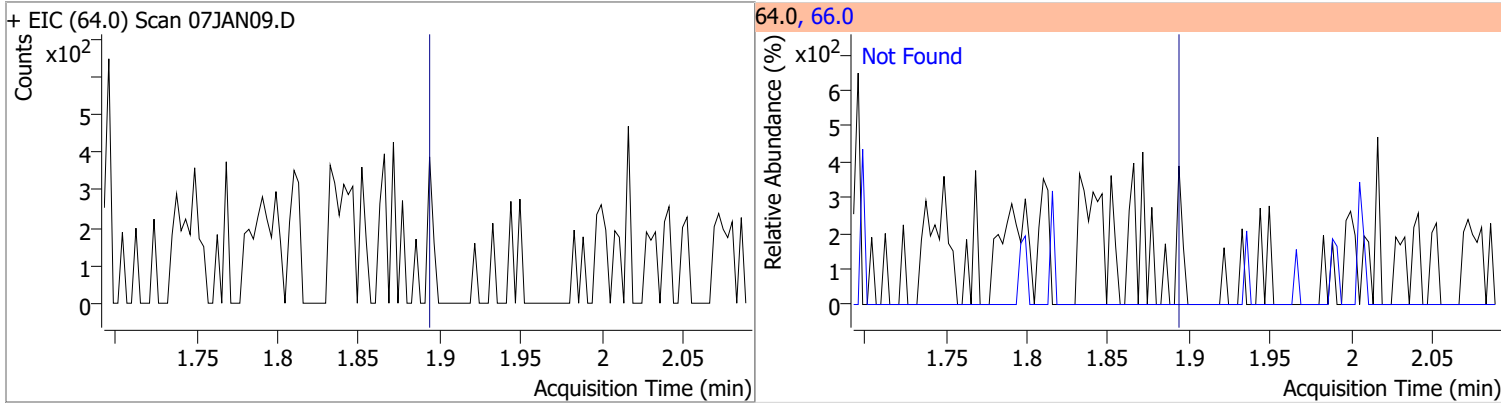


| Compound               | Conc. | Exp RT | QIon  | Exp Ratio |
|------------------------|-------|--------|-------|-----------|
| Trichlorofluoromethane | N.D.  | 2.14   | 103.0 | 64.2      |

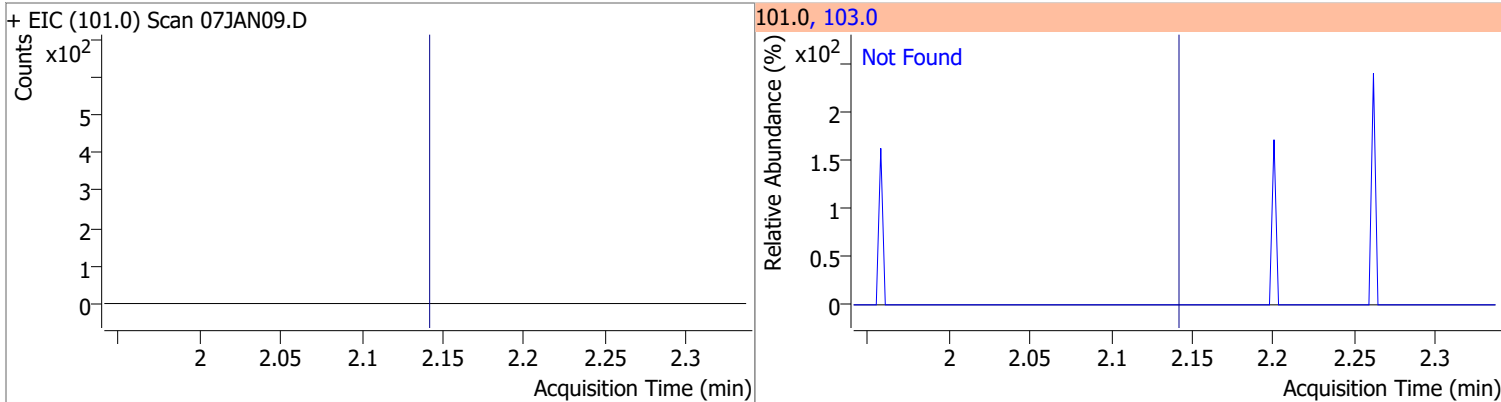

| Compound           | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethene | N.D.  | 2.70   | 61.0 | 180.3     | 63.0 | 56.7      |

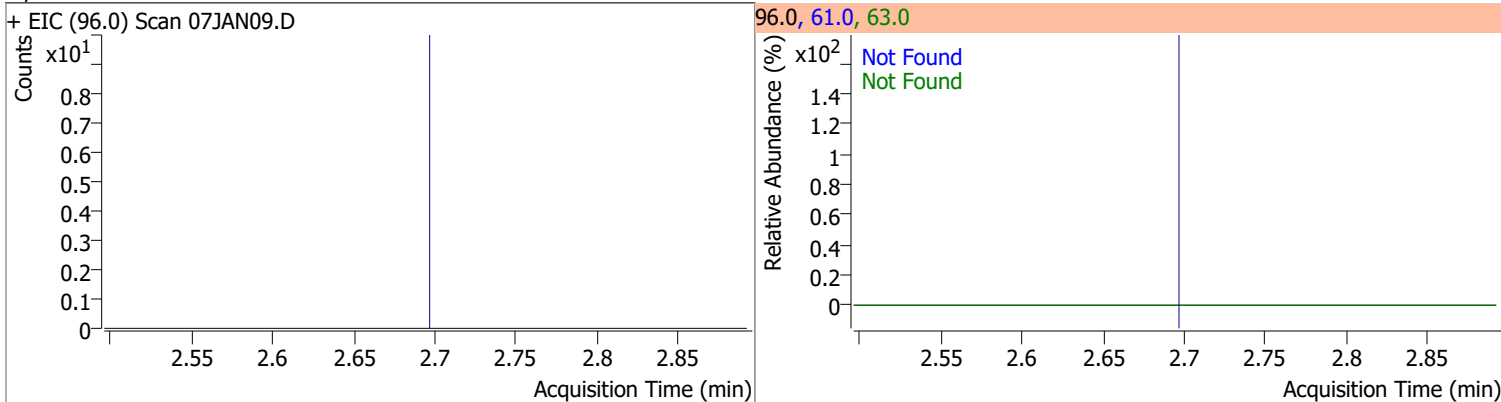


| Compound           | Conc.  | RT   | Dev(Min) | Resp.    | QIon | QRatio | Lower | Upper |
|--------------------|--------|------|----------|----------|------|--------|-------|-------|
| Methylene chloride | 2.2061 | 3.33 | -0.01    | 2658 (m) | 84.0 | 68.4   | 36.9  | 96.9  |
|                    |        |      |          |          | 86.0 | 42.8   | 14.3  | 74.3  |




# Quantitation Results Report (QT Reviewed)


| Compound                 | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,2-Dichloroethene | N.D.  | 3.72   | 61.0 | 153.9     | 98.0 | 65.7      |

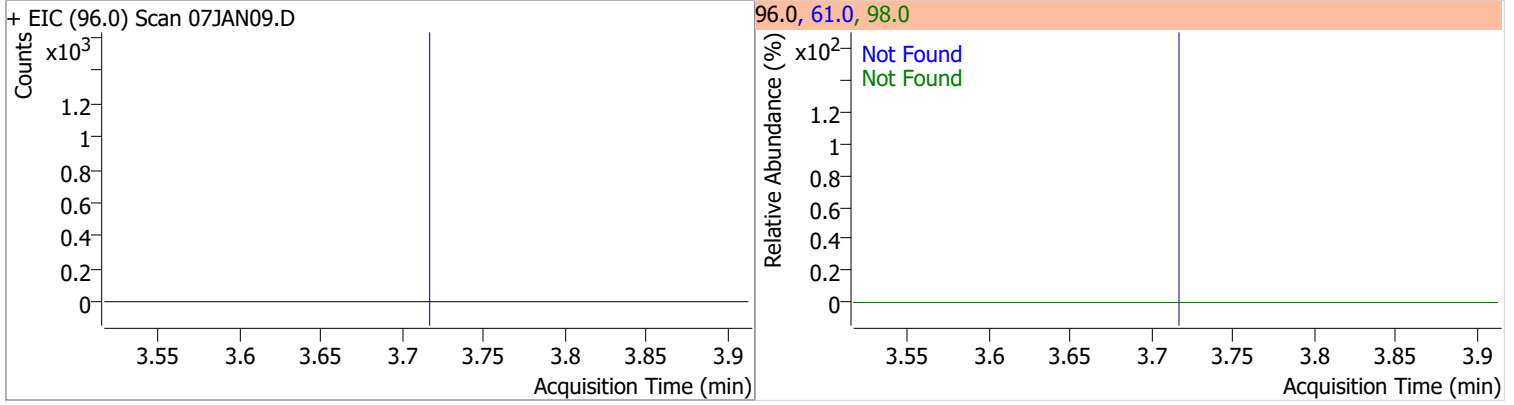


| Compound                       | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------------------|-------|--------|------|-----------|
| Methyl tert-butyl ether (MTBE) | N.D.  | 3.75   | 57.0 | 24.6      |

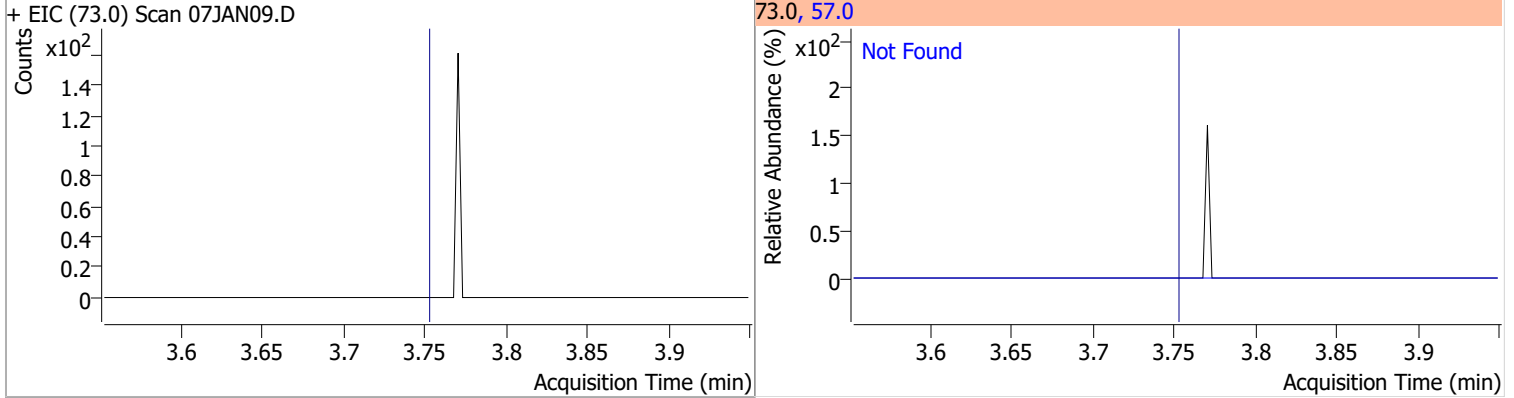

| Compound           | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethane | N.D.  | 4.38   | 65.0 | 32.1      | 83.0 | 13.7      |

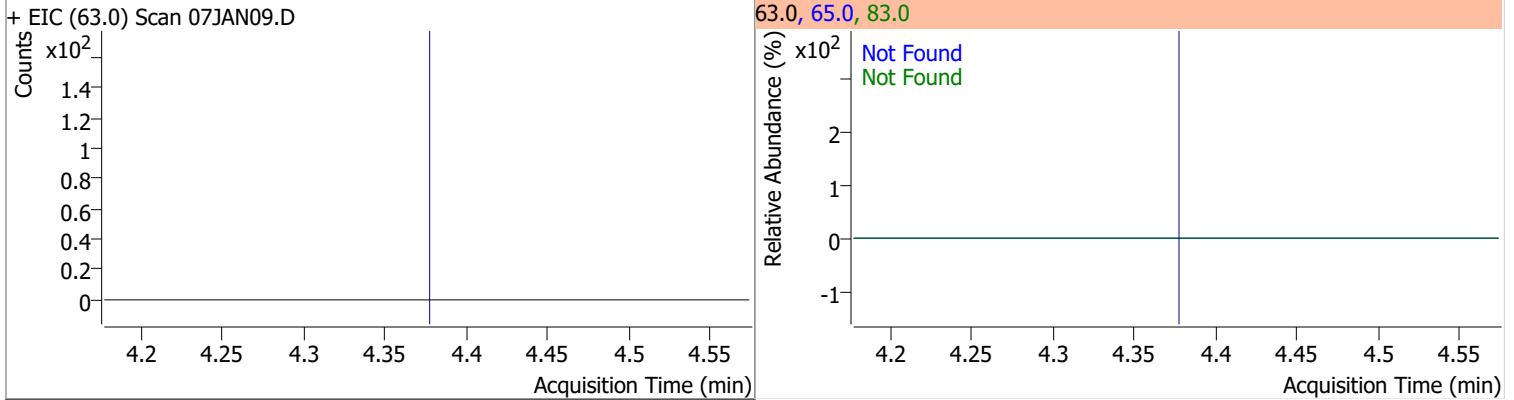


| Compound            | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|------|-----------|
| 2,2-Dichloropropane | N.D.  | 5.20   | 41.0 | 66.5      | 97.0 | 23.2      |

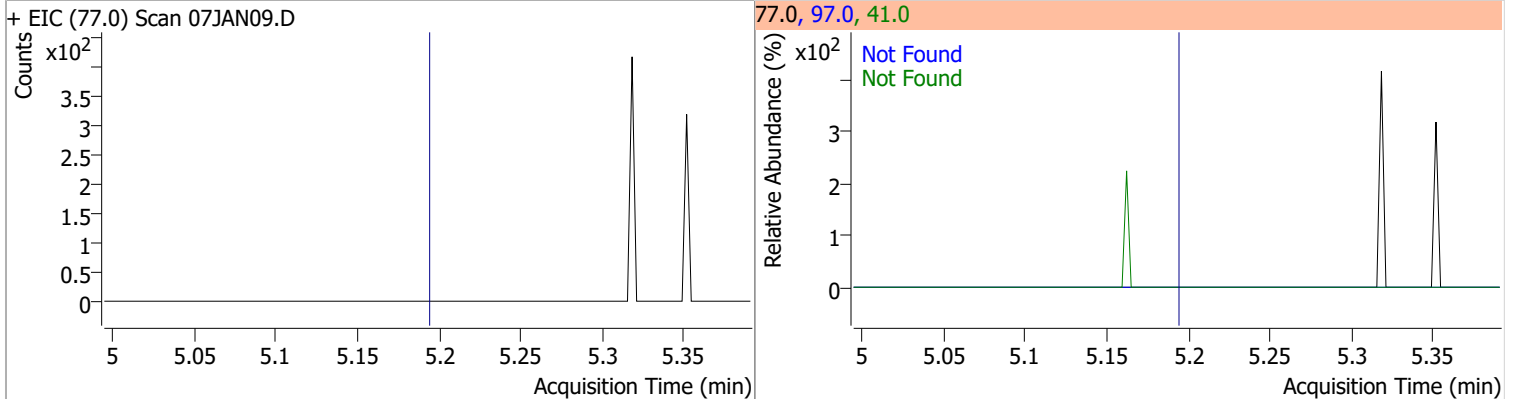


# Quantitation Results Report (QT Reviewed)


| Compound               | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|------------------------|-------|--------|------|-----------|------|-----------|
| cis-1,2-Dichloroethene | N.D.  | 5.22   | 61.0 | 167.2     | 98.0 | 67.3      |




| Compound            | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| Methyl ethyl ketone | N.D.  | 5.28   | 72.0 | 21.3      |







| Compound           | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|
| Bromochloromethane | N.D.  | 5.52   | 49.0 | 182.9     |



| Compound   | Conc.  | RT   | Dev(Min) | Resp.   | QIon | QRatio | Lower | Upper |
|------------|--------|------|----------|---------|------|--------|-------|-------|
| Chloroform | 0.2466 | 5.65 | 0.00     | 381 (m) | 85.0 | 65.6   | 36.0  | 96.0  |




# Quantitation Results Report (QT Reviewed)

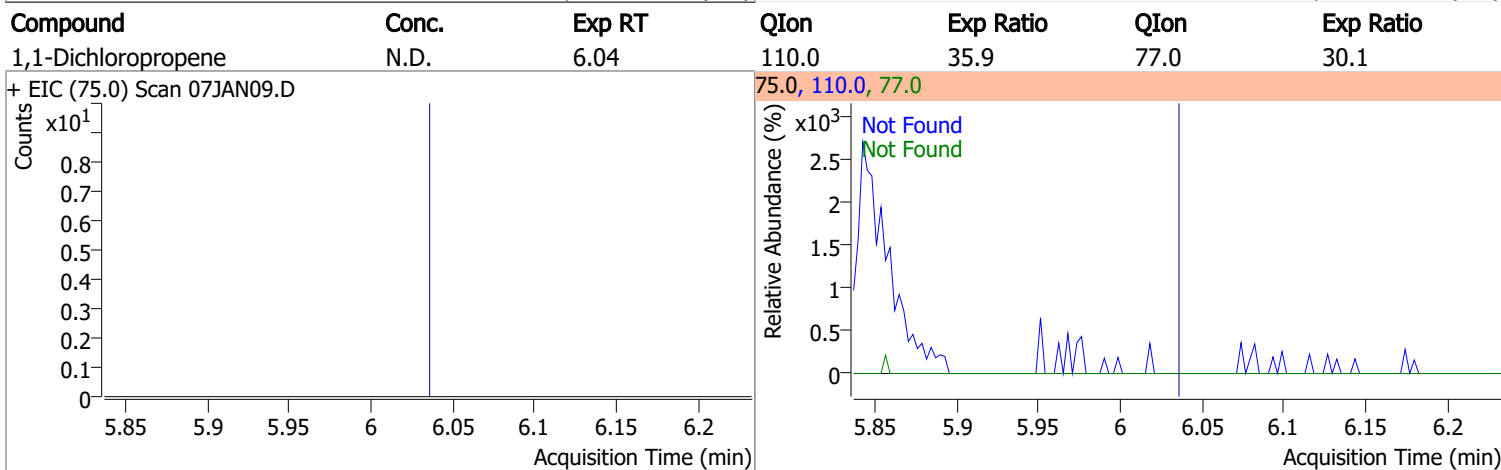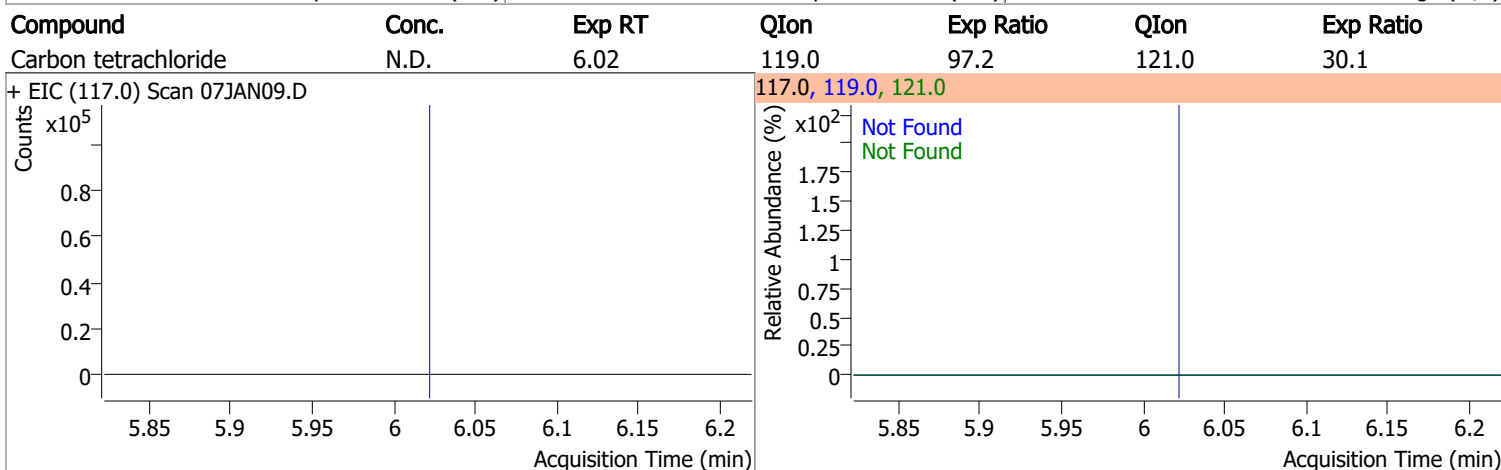


# Quantitation Results Report (QT Reviewed)


| Compound              | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 281.5597 | 6.23 | 0.00     | 92974 | 65.0 | 192.3  | 166.5 | 226.5 |

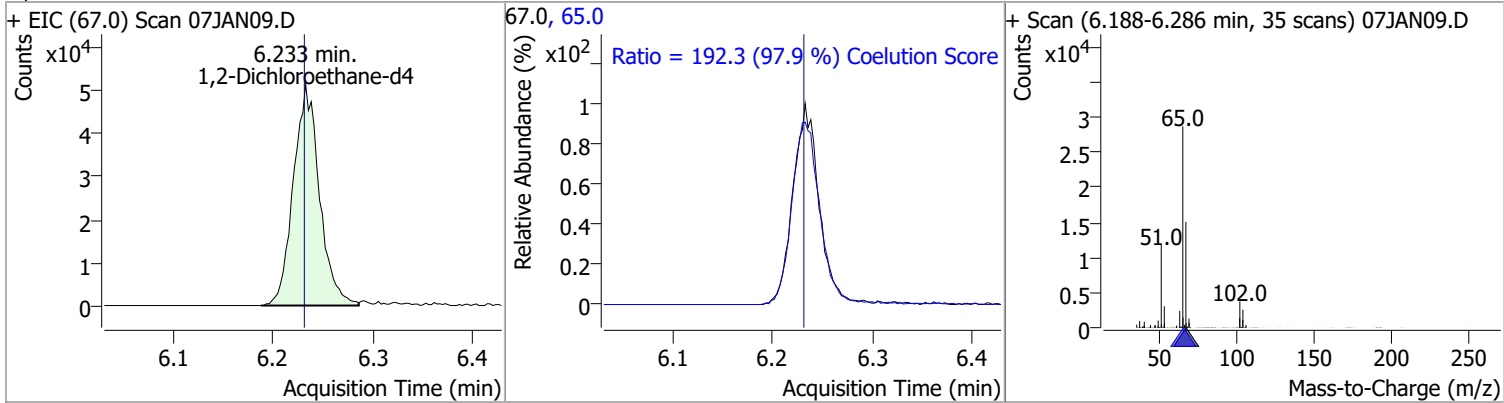


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------|-------|--------|------|-----------|
| Benzene  | N.D.  | 6.28   | 77.0 | 23.5      |

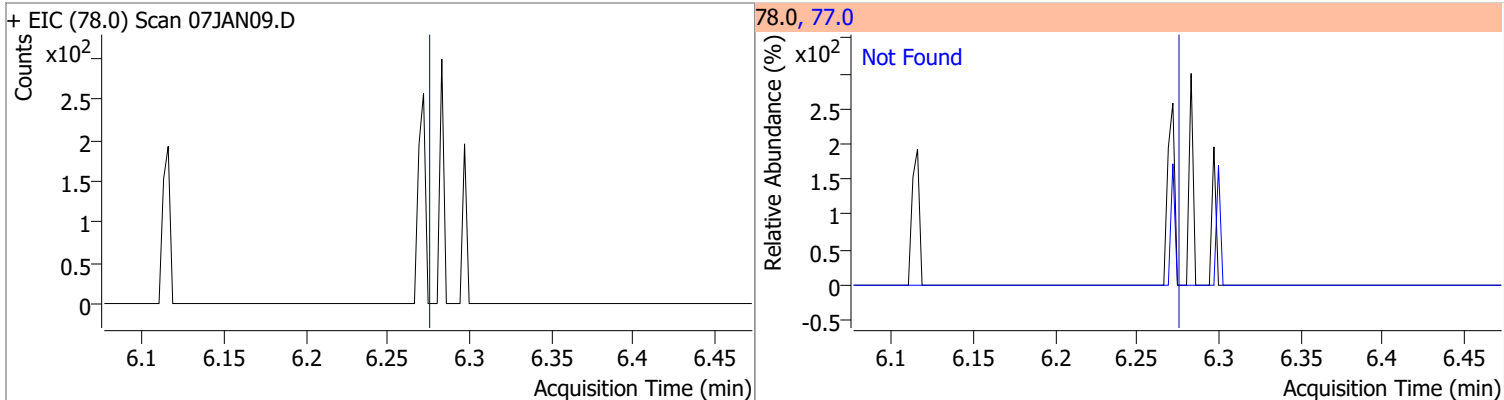





| Compound           | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,2-Dichloroethane | N.D.  | 6.32   | 64.0 | 29.9      | 98.0 | 7.6       |

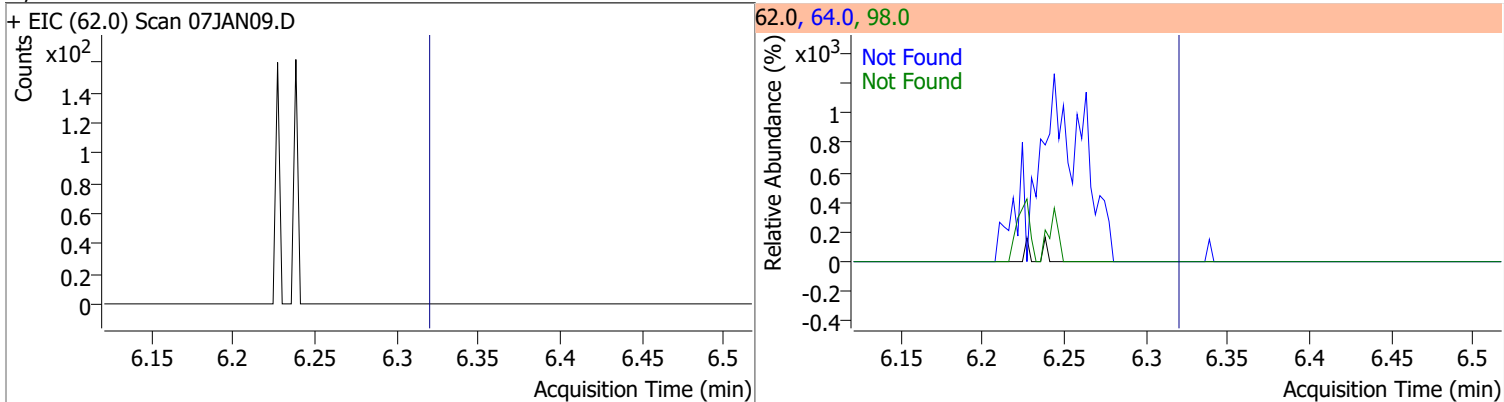

| Compound        | Conc. | Exp RT | QIon  | Exp Ratio | QIon | Exp Ratio |
|-----------------|-------|--------|-------|-----------|------|-----------|
| Trichloroethene | N.D.  | 7.03   | 130.0 | 101.5     | 97.0 | 64.1      |

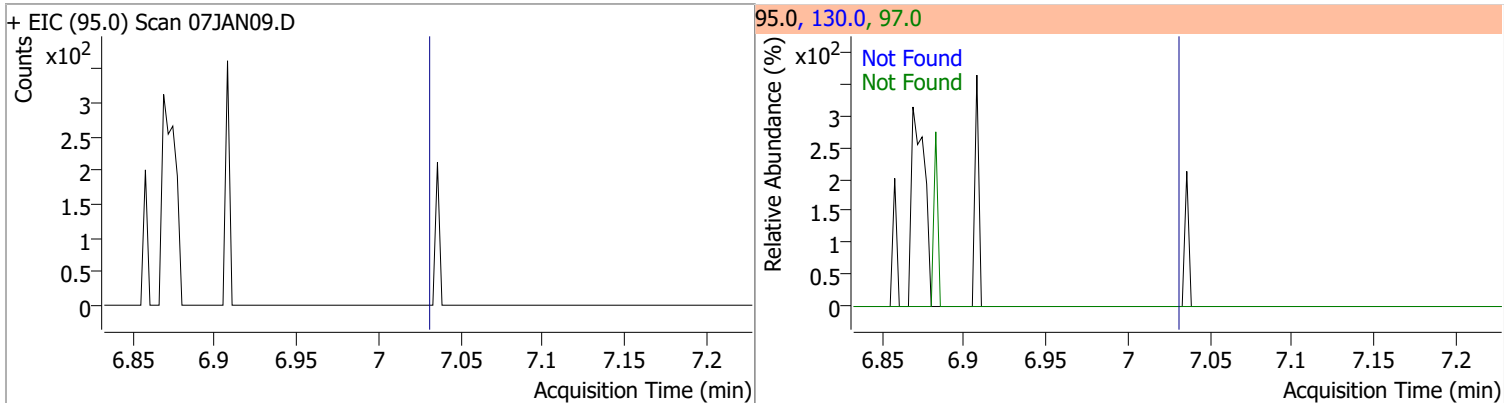


# Quantitation Results Report (QT Reviewed)

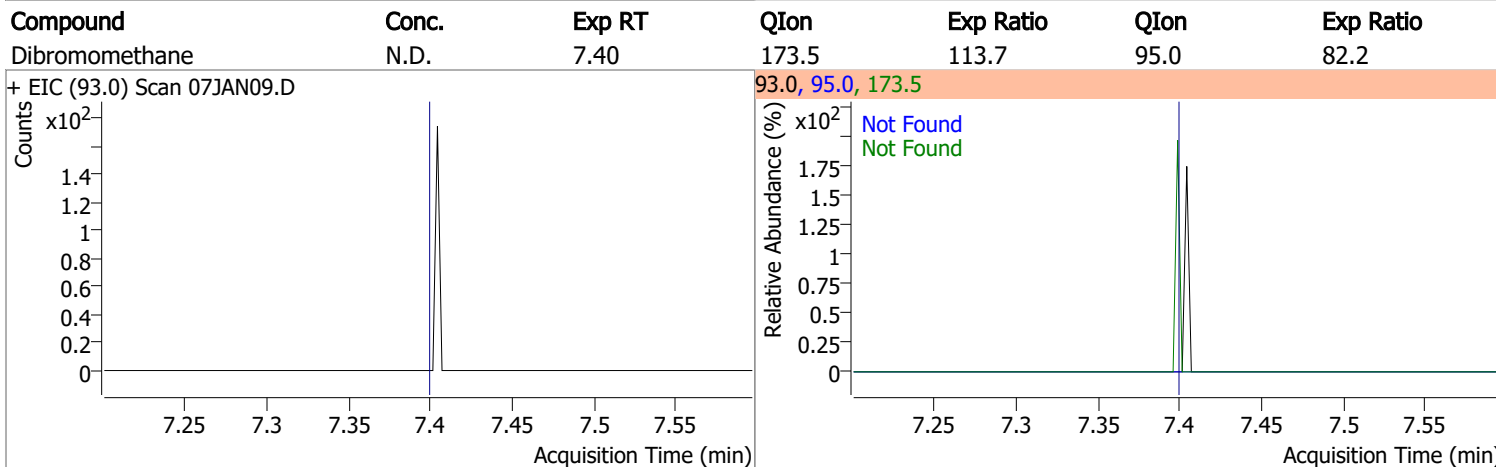


# Quantitation Results Report (QT Reviewed)


| Compound   | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 271.9136 | 8.32 | 0.00     | 816456 | 100.0 | 63.4   | 34.4  | 94.4  |
|            |          |      |          |        | 99.0  | 9.6    | 0.0   | 39.6  |

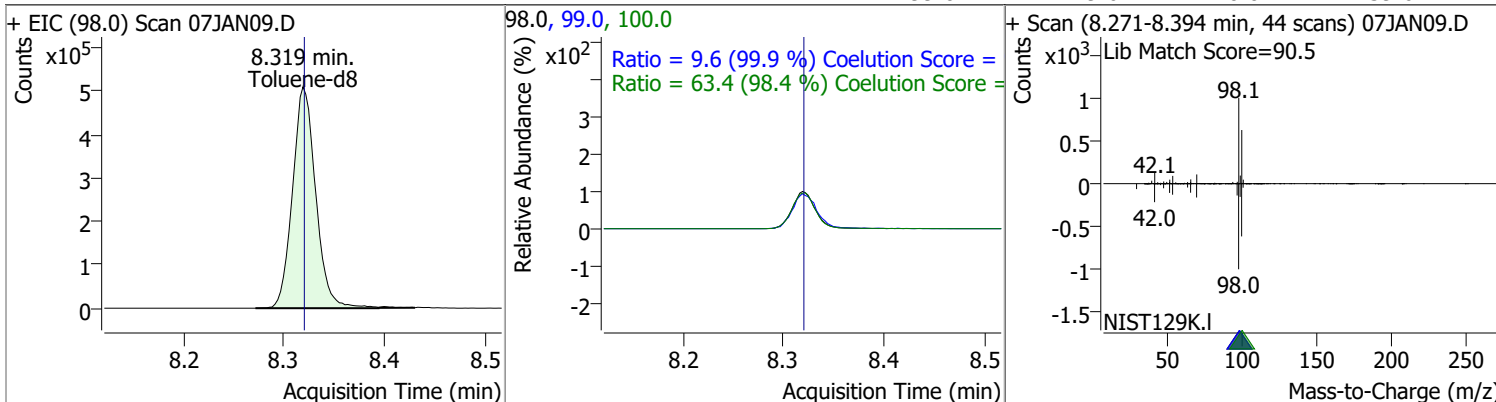


| Compound | Conc.  | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|--------|------|----------|-------|------|--------|-------|-------|
| Toluene  | 2.1950 | 8.39 | 0.00     | 4452  | 91.0 | 175.0  | 145.8 | 205.8 |

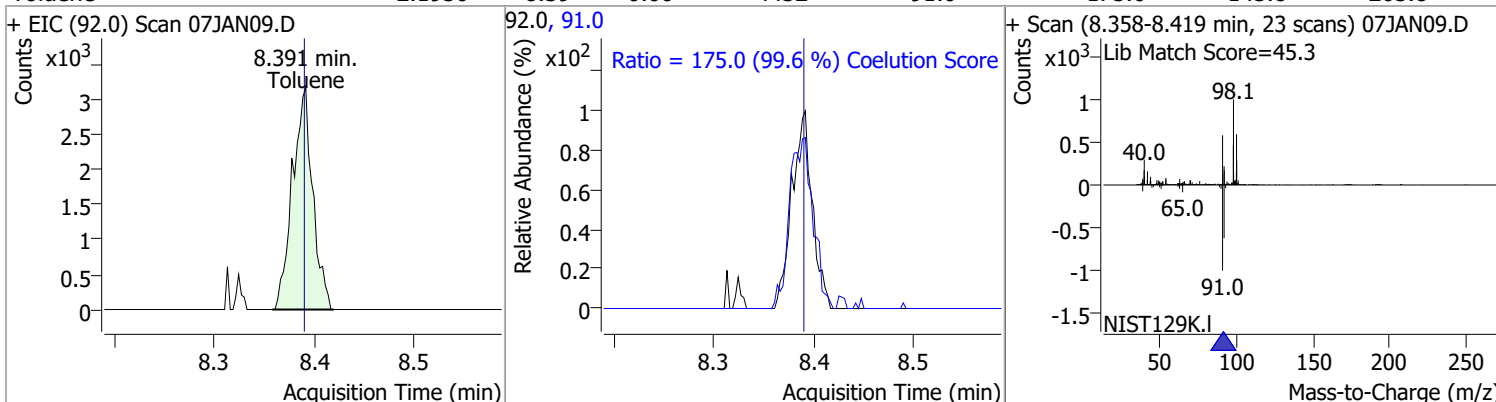









| Compound                  | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,3-Dichloropropene | N.D.  | 8.64   | 39.0 | 53.4      | 77.0 | 32.4      |

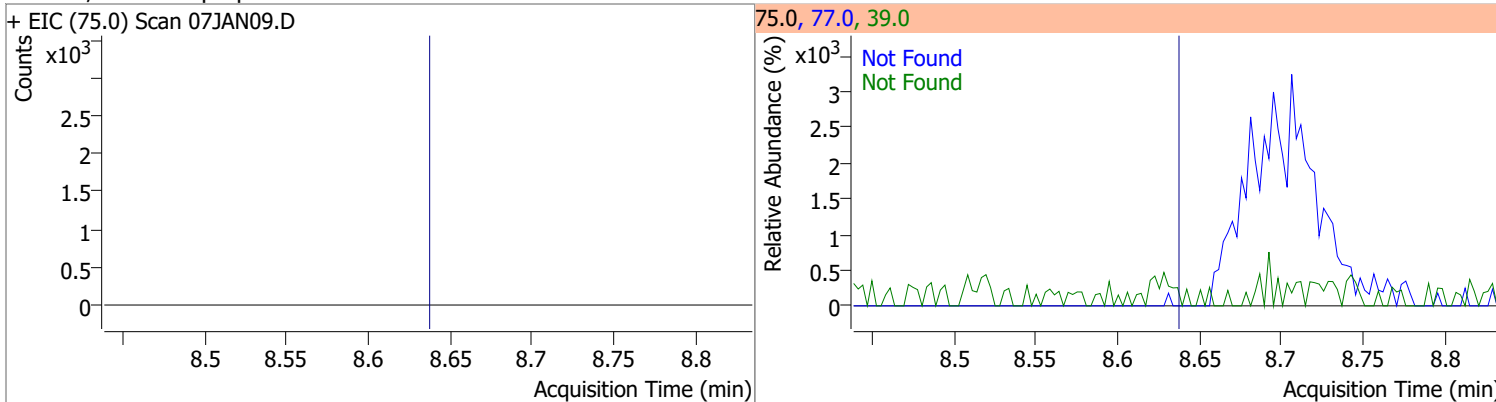

| Compound              | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------------|-------|--------|------|-----------|------|-----------|
| 1,1,2-Trichloroethane | N.D.  | 8.82   | 97.0 | 114.6     | 85.0 | 67.6      |








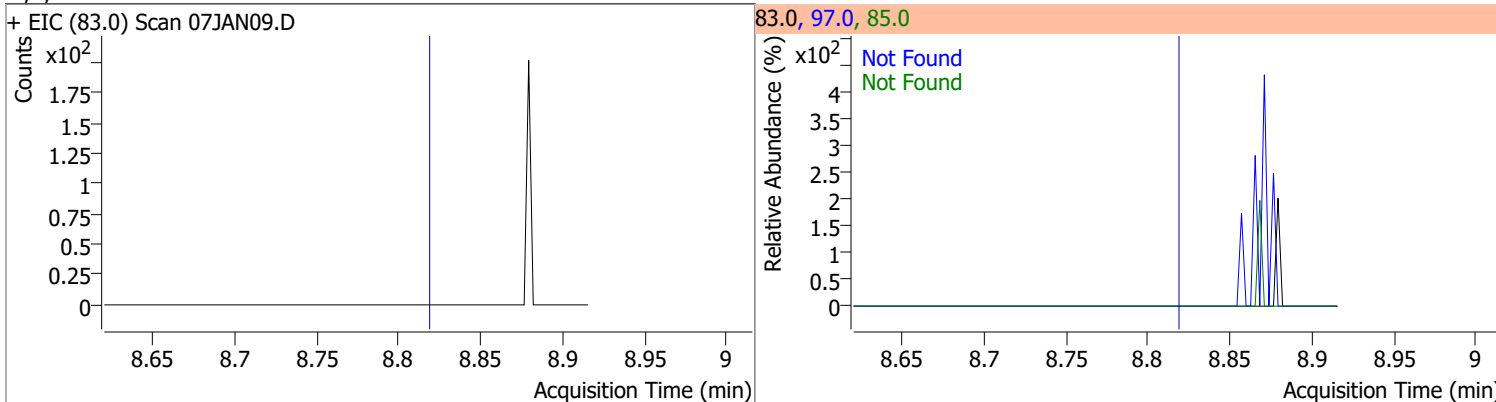


# Quantitation Results Report (QT Reviewed)
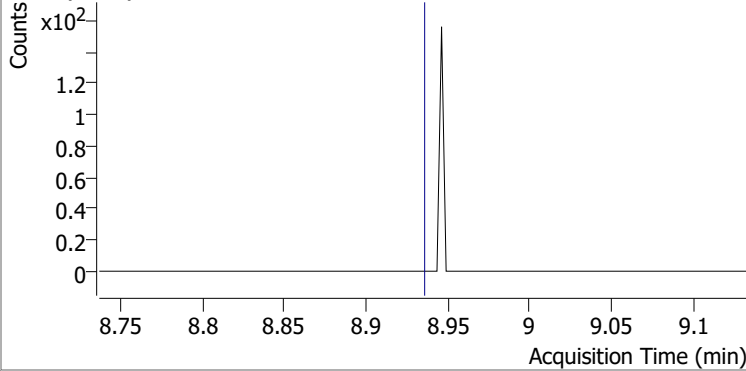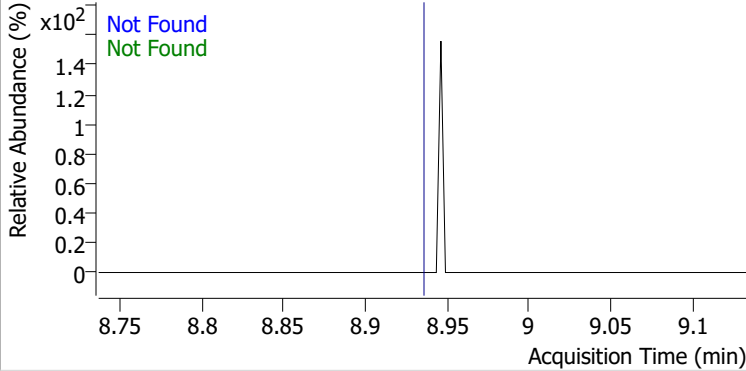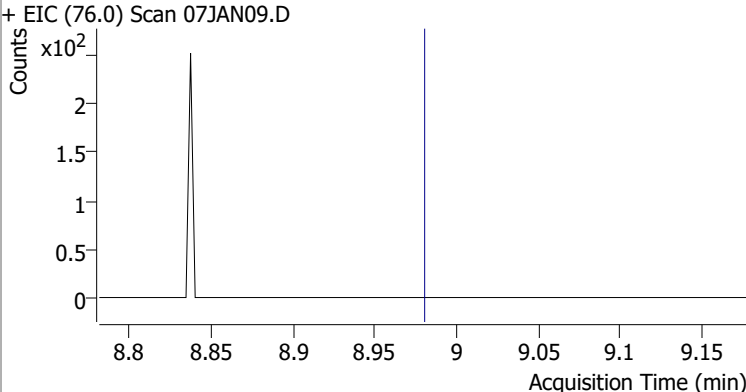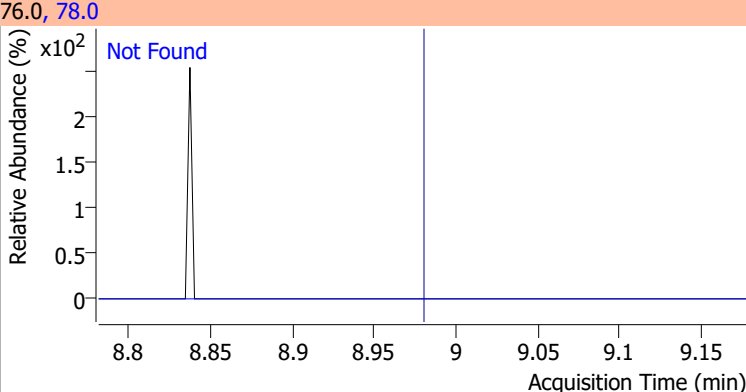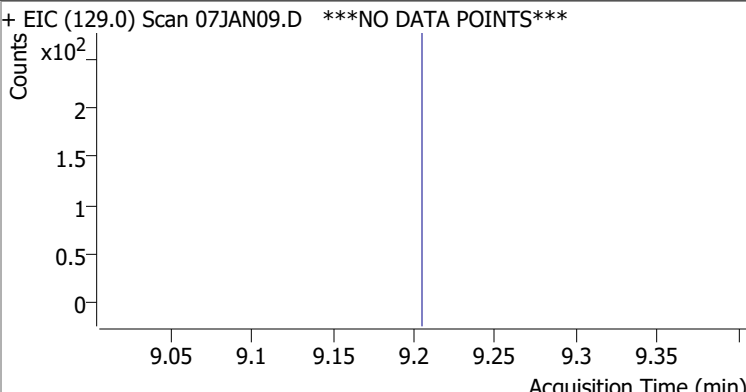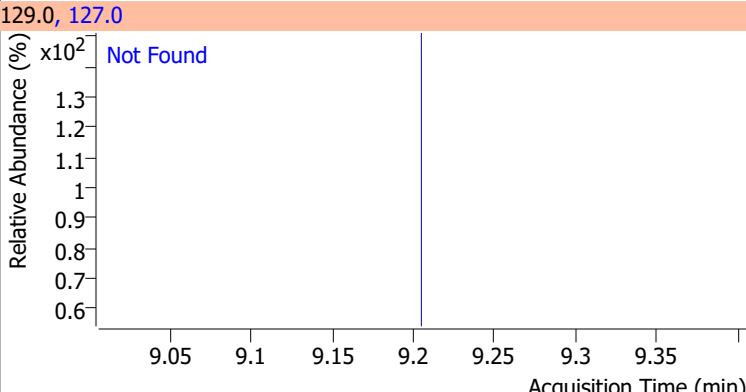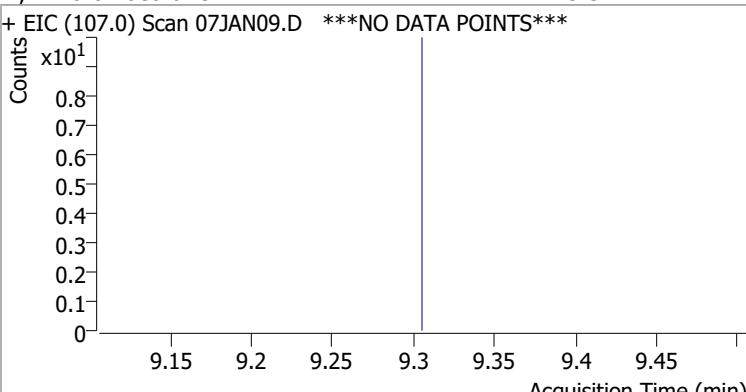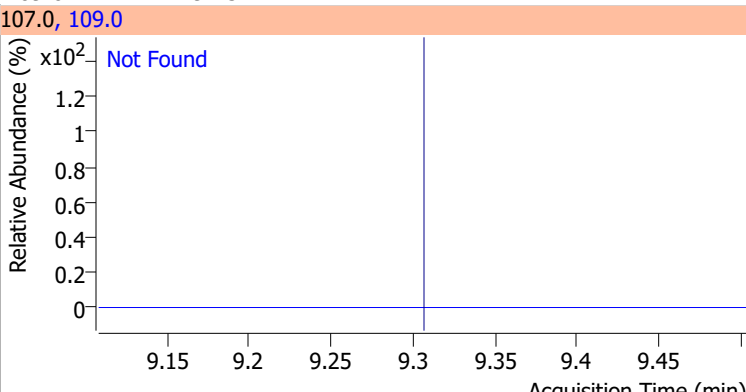
| Compound                                                                           | Conc. | Exp RT | QIon                                                                                 | Exp Ratio | QIon  | Exp Ratio |
|------------------------------------------------------------------------------------|-------|--------|--------------------------------------------------------------------------------------|-----------|-------|-----------|
| Tetrachloroethene                                                                  | N.D.  | 8.94   | 165.8                                                                                | 128.6     | 129.0 | 91.5      |
| + EIC (163.8) Scan 07JAN09.D                                                       |       |        | 163.8, 129.0, 165.8                                                                  |           |       |           |
|    |       |        |    |           |       |           |
| 1,3-Dichloropropane                                                                | N.D.  | 8.98   | 78.0                                                                                 | 32.9      |       |           |
| + EIC (76.0) Scan 07JAN09.D                                                        |       |        | 76.0, 78.0                                                                           |           |       |           |
|   |       |        |   |           |       |           |
| Chlorodibromomethane                                                               | N.D.  | 9.21   | 127.0                                                                                | 78.0      |       |           |
| + EIC (129.0) Scan 07JAN09.D ***NO DATA POINTS***                                  |       |        | 129.0, 127.0                                                                         |           |       |           |
|  |       |        |  |           |       |           |
| 1,2-Dibromoethane                                                                  | N.D.  | 9.31   | 109.0                                                                                | 94.5      |       |           |
| + EIC (107.0) Scan 07JAN09.D ***NO DATA POINTS***                                  |       |        | 107.0, 109.0                                                                         |           |       |           |
|  |       |        |  |           |       |           |




# Quantitation Results Report (QT Reviewed)

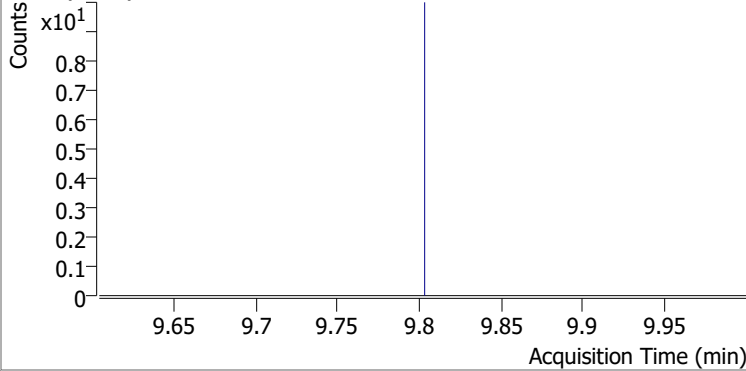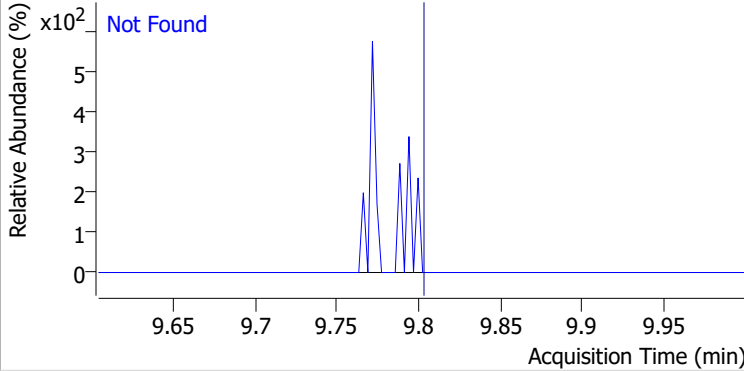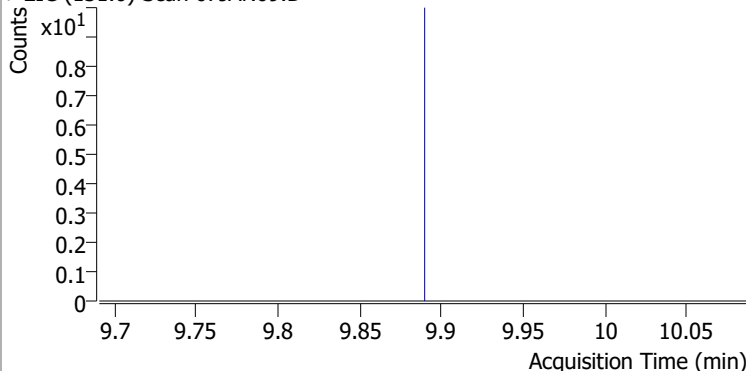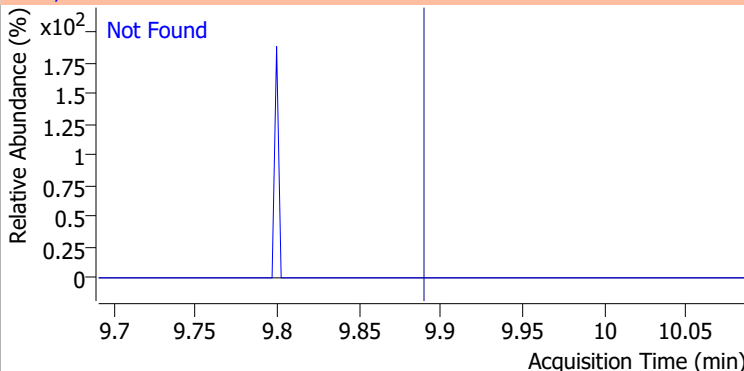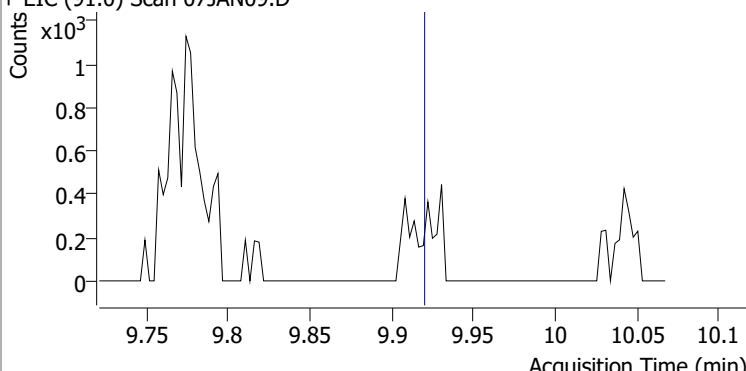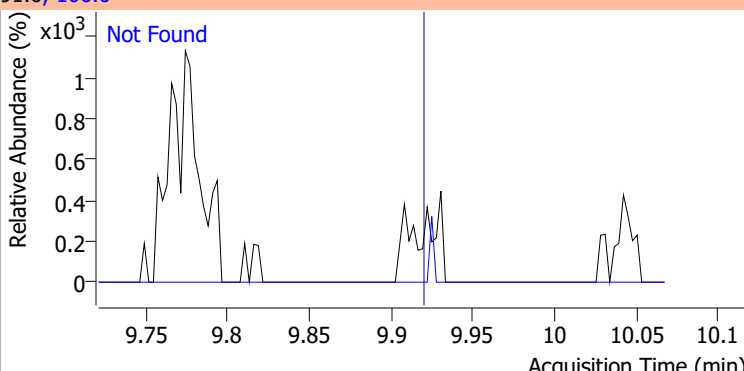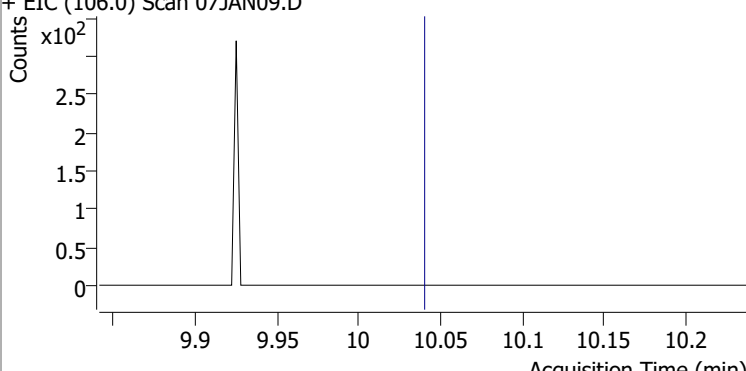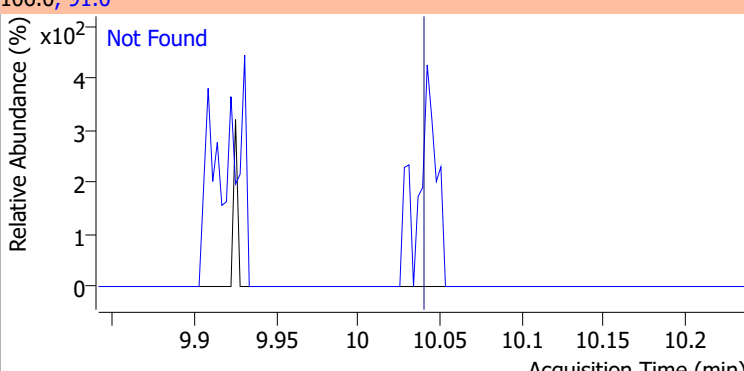
| Compound                                                                           | Conc. | Exp RT | QIon                                                                                 | Exp Ratio |
|------------------------------------------------------------------------------------|-------|--------|--------------------------------------------------------------------------------------|-----------|
| Chlorobenzene                                                                      | N.D.  | 9.80   | 114.0                                                                                | 32.1      |
| + EIC (112.0) Scan 07JAN09.D                                                       |       |        | 112.0, 114.0                                                                         |           |
|    |       |        |    |           |
| 1,1,1,2-Tetrachloroethane                                                          | N.D.  | 9.89   | 133.0                                                                                | 98.6      |
| + EIC (131.0) Scan 07JAN09.D                                                       |       |        | 131.0, 133.0                                                                         |           |
|   |       |        |   |           |
| Ethylbenzene                                                                       | N.D.  | 9.92   | 106.0                                                                                | 31.1      |
| + EIC (91.0) Scan 07JAN09.D                                                        |       |        | 91.0, 106.0                                                                          |           |
|  |       |        |  |           |
| m+p-Xylenes                                                                        | N.D.  | 10.04  | 91.0                                                                                 | 201.4     |
| + EIC (106.0) Scan 07JAN09.D                                                       |       |        | 106.0, 91.0                                                                          |           |
|  |       |        |  |           |

# Quantitation Results Report (QT Reviewed)


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------|-------|--------|------|-----------|
| o-Xylene | N.D.  | 10.43  | 91.0 | 213.1     |

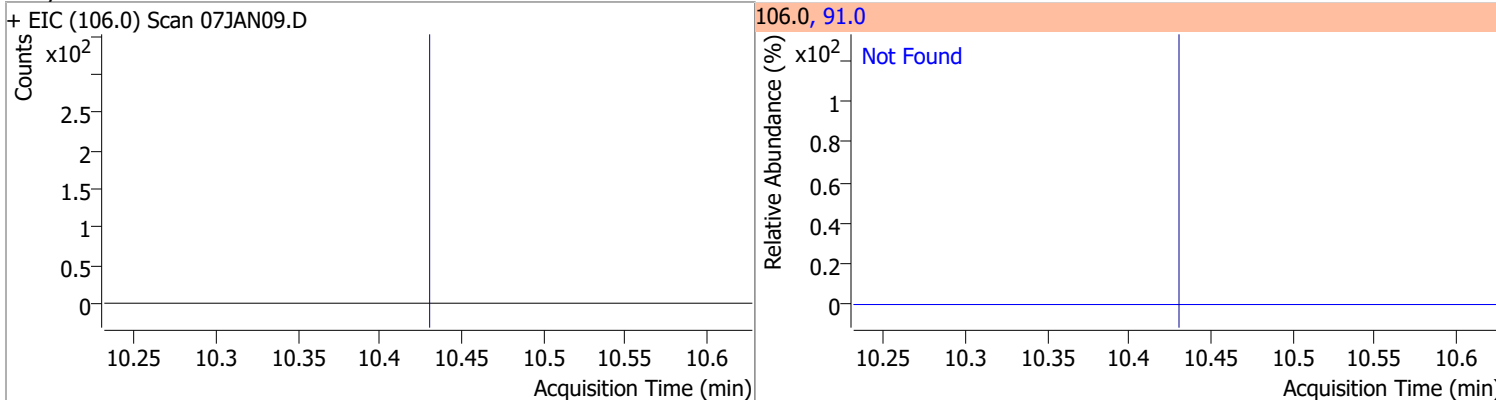


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------|-------|--------|------|-----------|
| Styrene  | N.D.  | 10.45  | 78.0 | 49.6      |

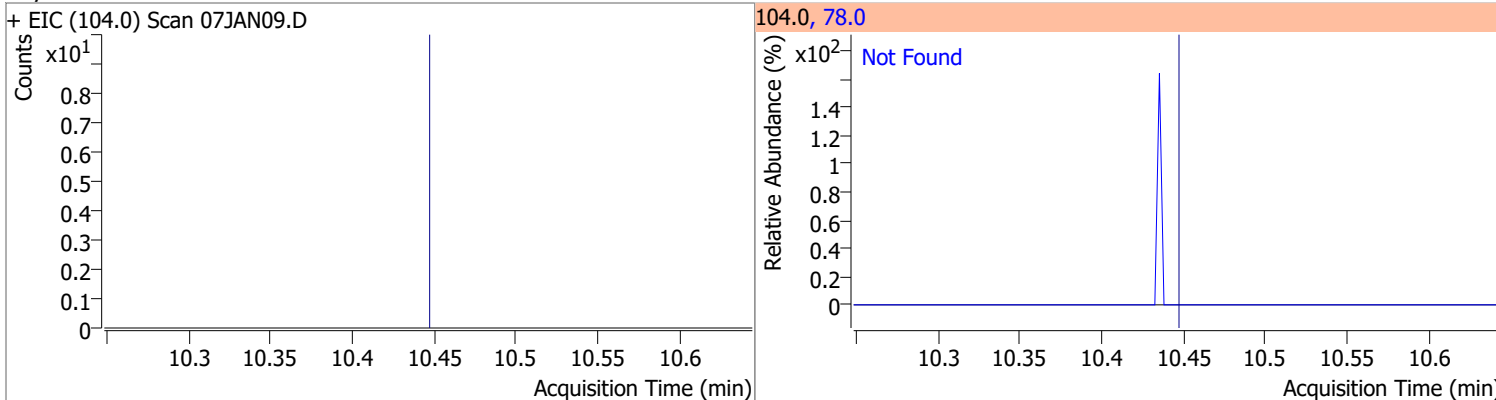

| Compound  | Conc. | Exp RT | QIon  | Exp Ratio | QIon  | Exp Ratio |
|-----------|-------|--------|-------|-----------|-------|-----------|
| Bromoform | N.D.  | 10.63  | 170.5 | 52.1      | 174.5 | 50.1      |

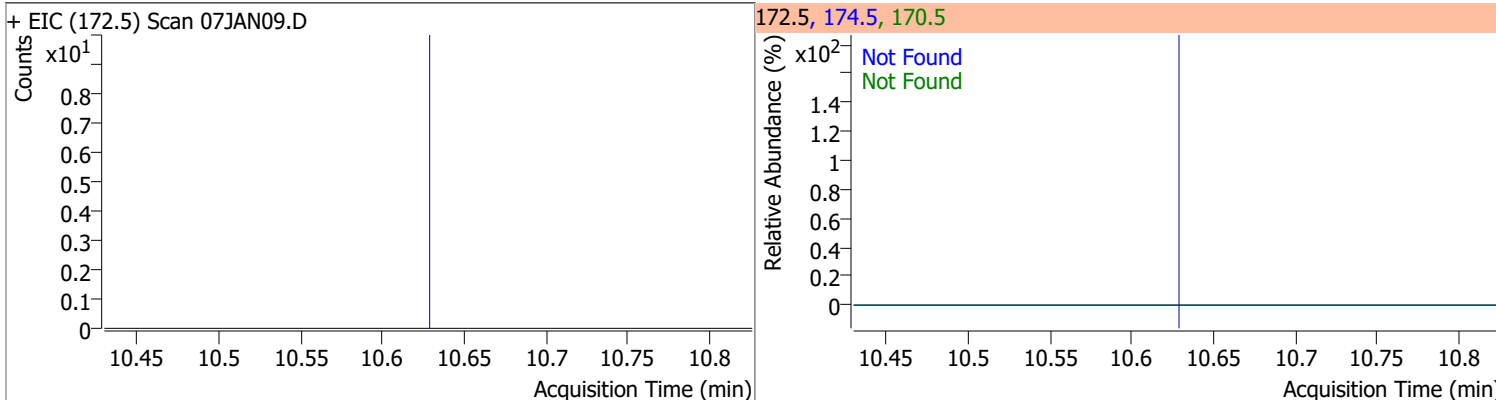









| Compound             | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 270.7711 | 10.95 | 0.00     | 234685 | 174.0 | 94.4   | 61.7  | 121.7 |
|                      |          |       |          |        | 176.0 | 91.6   | 60.6  | 120.6 |

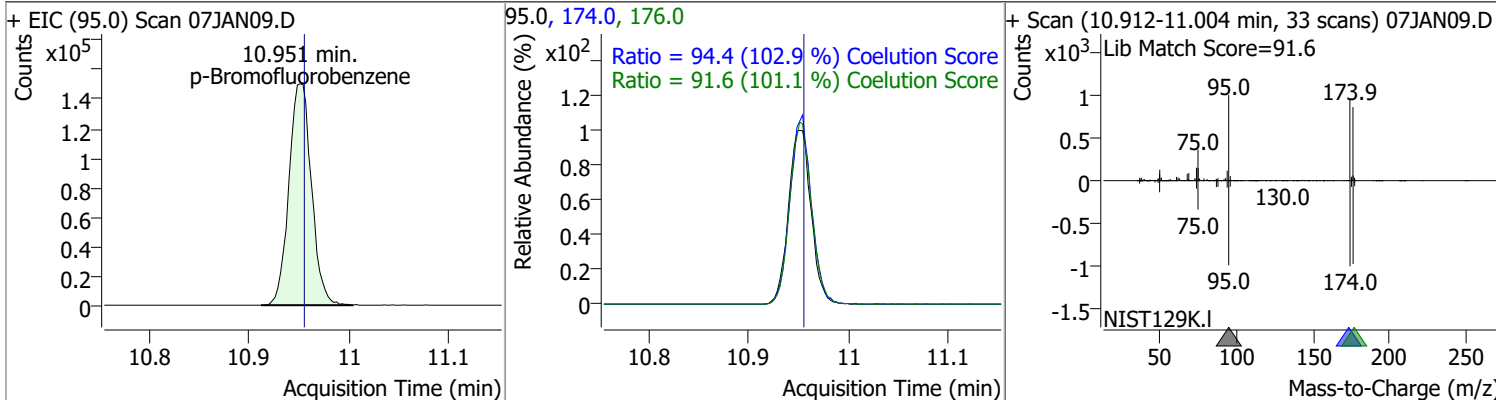

# Quantitation Results Report (QT Reviewed)


| Compound                     | Conc. | Exp RT | QIon               | Exp Ratio | QIon  | Exp Ratio |
|------------------------------|-------|--------|--------------------|-----------|-------|-----------|
| Bromobenzene                 | N.D.  | 11.09  | 77.0               | 145.7     | 158.0 | 96.5      |
| + EIC (156.0) Scan 07JAN09.D |       |        | 156.0, 77.0, 158.0 |           |       |           |
|                              |       |        |                    |           |       |           |
| 1,1,2,2-Tetrachloroethane    | N.D.  | 11.12  | 85.0               | 66.2      |       |           |
| + EIC (83.0) Scan 07JAN09.D  |       |        | 83.0, 85.0         |           |       |           |
|                              |       |        |                    |           |       |           |
| 1,2,3-Trichloropropane       | N.D.  | 11.15  | 112.0              | 63.5      |       |           |
| + EIC (110.0) Scan 07JAN09.D |       |        | 110.0, 112.0       |           |       |           |
|                              |       |        |                    |           |       |           |
| 2-Chlorotoluene              | N.D.  | 11.29  | 91.0               | 282.3     |       |           |
| + EIC (126.0) Scan 07JAN09.D |       |        | 126.0, 91.0        |           |       |           |
|                              |       |        |                    |           |       |           |

# Quantitation Results Report (QT Reviewed)
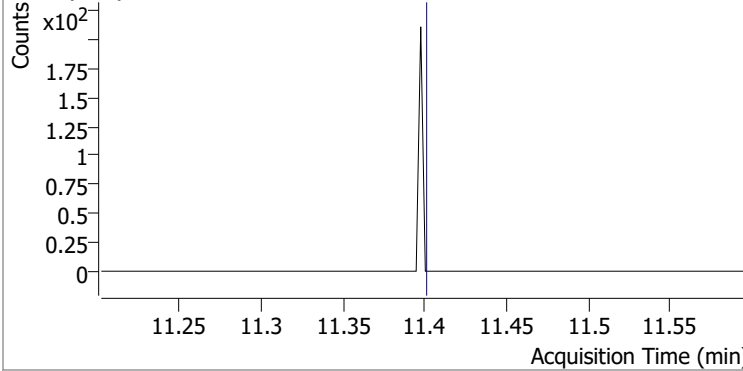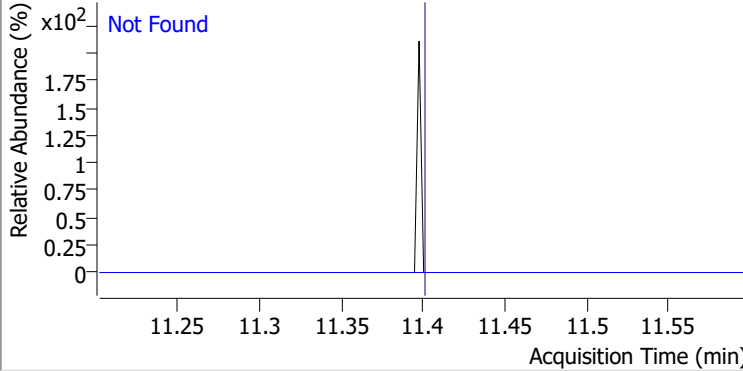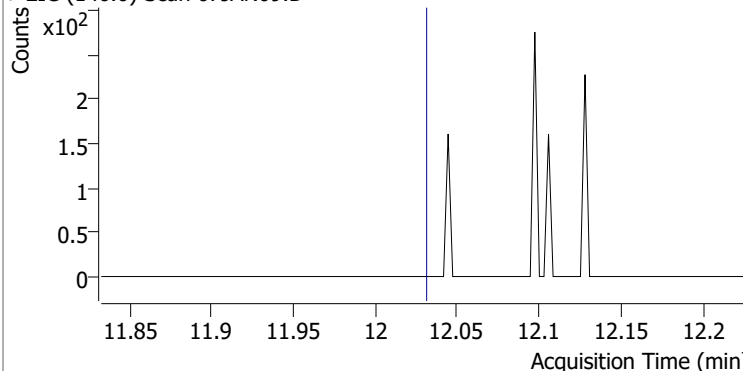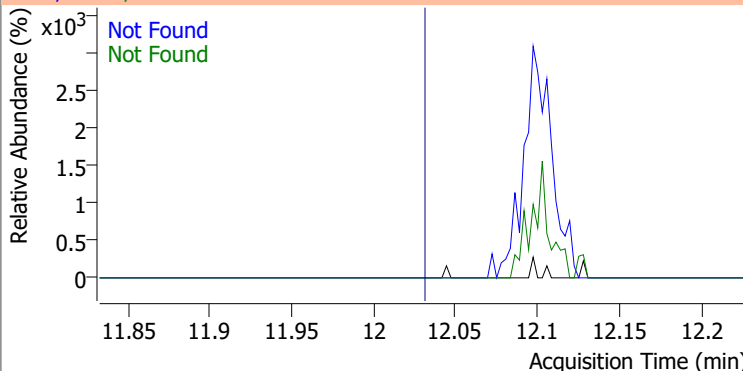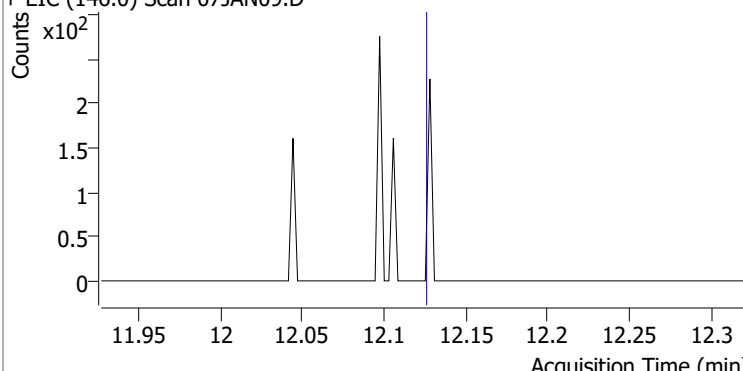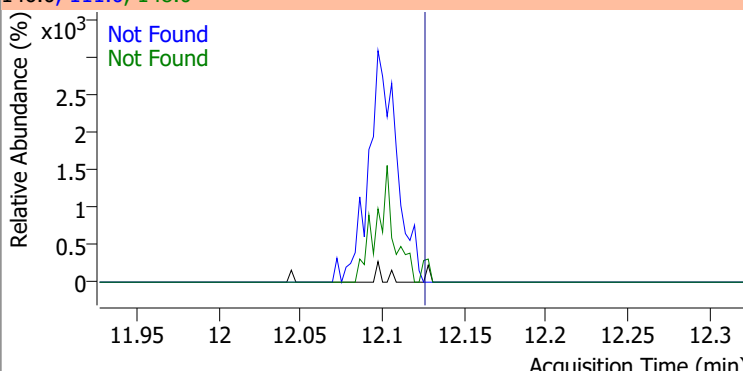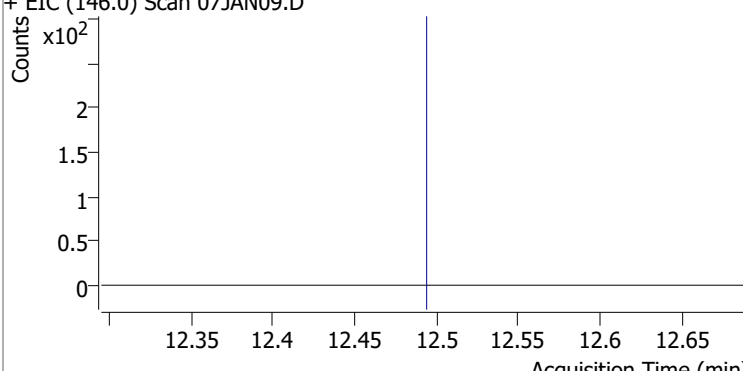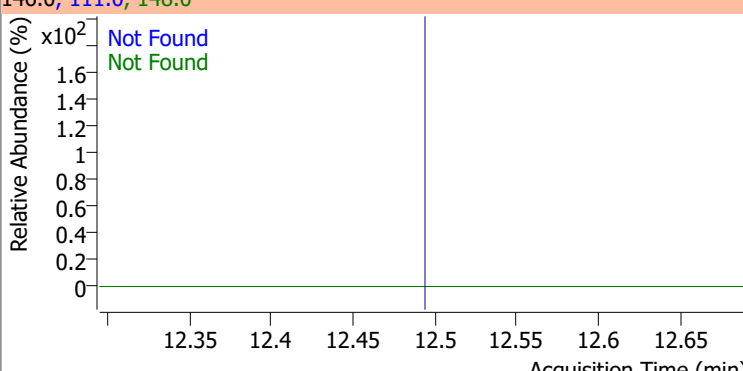
| Compound                                                                           | Conc. | Exp RT | QIon                                                                                 | Exp Ratio |      |           |
|------------------------------------------------------------------------------------|-------|--------|--------------------------------------------------------------------------------------|-----------|------|-----------|
| 4-Chlorotoluene                                                                    | N.D.  | 11.40  | 126.0                                                                                | 31.7      |      |           |
| + EIC (91.0) Scan 07JAN09.D                                                        |       |        | 91.0, 126.0                                                                          |           |      |           |
|    |       |        |    |           |      |           |
| 1,3-Dichlorobenzene                                                                | N.D.  | 12.03  | 148.0                                                                                | 63.6      | QIon | Exp Ratio |
| + EIC (146.0) Scan 07JAN09.D                                                       |       |        | 146.0, 111.0, 148.0                                                                  |           |      |           |
|   |       |        |   |           |      |           |
| 1,4-Dichlorobenzene                                                                | N.D.  | 12.13  | 148.0                                                                                | 63.1      | QIon | Exp Ratio |
| + EIC (146.0) Scan 07JAN09.D                                                       |       |        | 146.0, 111.0, 148.0                                                                  |           |      |           |
|  |       |        |  |           |      |           |
| 1,2-Dichlorobenzene                                                                | N.D.  | 12.49  | 148.0                                                                                | 63.9      | QIon | Exp Ratio |
| + EIC (146.0) Scan 07JAN09.D                                                       |       |        | 146.0, 111.0, 148.0                                                                  |           |      |           |
|  |       |        |  |           |      |           |

# Quantitation Results Report (QT Reviewed)

|                |                                     |                   |                       |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File      | 07JAN10.D                           | Operator          | MSC                   |
| Acq. Method    | 5975CACQF.M                         | Acq. Date-Time    | 1/7/2022 1:46:47 PM   |
| Sample Name    | B22010214-002A                      | Instrument        | VOA5975C              |
| Vial           | 10                                  | Multiplier        | 1.00                  |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m  | Comment           |                       |
| Tune File      | BFB_Atune3.u                        | Tune Date         | 10/11/2021 4:02:00 PM |
| Batch Name     | VG010722_8260B.batch.bin            | Last Calib Update | 3/2/2022 10:41:44 AM  |
| Ref Library    | \\MASSHUNTER\Org\Library\NIST129K.I |                   |                       |

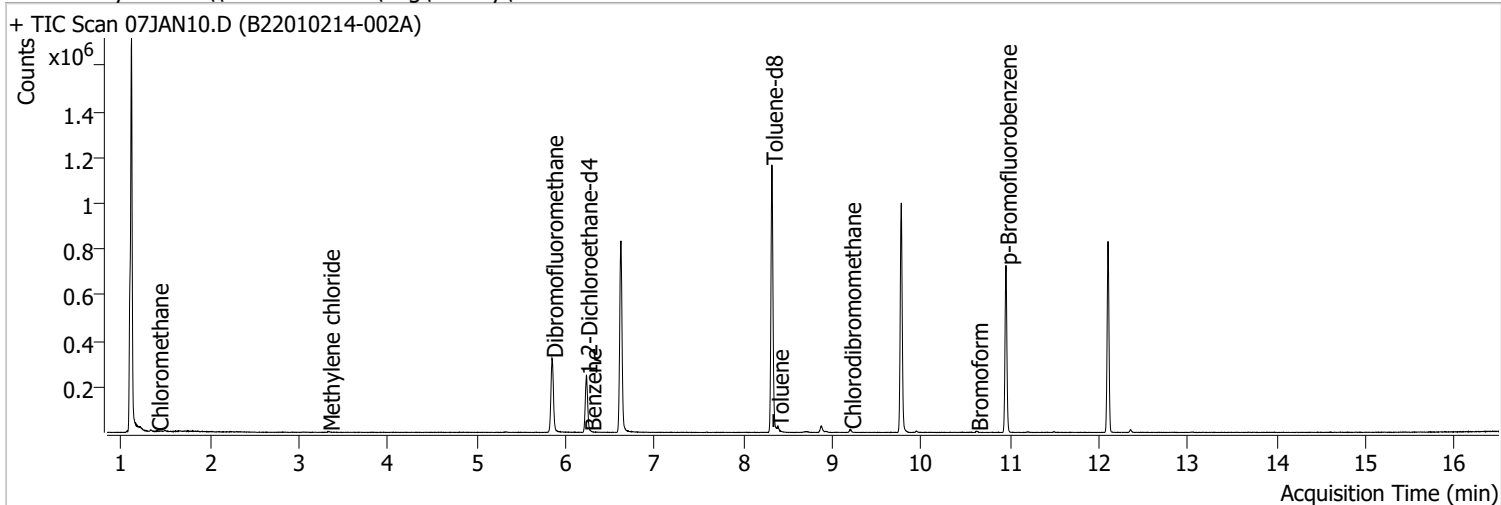

| Compound                           | RT                   | QIon  | Resp.  | Conc.                | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|----------------------|-------|----------|
| <b>Internal Standards</b>          |                      |       |        |                      |       |          |
| M Fluorobenzene                    | 6.621                | 96.0  | 710622 | 250.0000             | ng    | -0.003   |
| M Chlorobenzene-d5                 | 9.772                | 82.0  | 276679 | 250.0000             | ng    | 0.000    |
| M 1,4-Dichlorobenzene-d4           | 12.100               | 152.0 | 197130 | 250.0000             | ng    | 0.000    |
| <b>System Monitoring Compounds</b> |                      |       |        |                      |       |          |
| S Dibromofluoromethane             | 5.845                | 113.0 | 189885 | 283.6314             | ng    | 0.000    |
| Spiked Amount: 250.000             | Range: 80.0 - 119.0% |       |        | Recovery = 113.45%   |       |          |
| S 1,2-Dichloroethane-d4            | 6.233                | 67.0  | 88230  | 305.1186             | ng    | 0.000    |
| Spiked Amount: 250.000             | Range: 81.0 - 118.0% |       |        | Recovery = 122.05% * |       |          |
| S Toluene-d8                       | 8.319                | 98.0  | 699981 | 262.5368             | ng    | 0.000    |
| Spiked Amount: 250.000             | Range: 89.0 - 112.0% |       |        | Recovery = 105.01%   |       |          |
| S p-Bromofluorobenzene             | 10.951               | 95.0  | 203968 | 282.4305             | ng    | -0.003   |
| Spiked Amount: 250.000             | Range: 85.0 - 114.0% |       |        | Recovery = 112.97%   |       |          |
| <b>Target Compounds</b>            |                      |       |        |                      |       |          |
| T Dichlorodifluoromethane          | 0.000                |       | 0      | N.D.                 |       |          |
| T Chloromethane                    | 1.409                | 50.0  | 2332   | 2.0632               | ng    | 99       |
| T Vinyl chloride                   | 0.000                |       | 0      | N.D.                 |       |          |
| T Bromomethane                     | 0.000                |       | 0      | N.D.                 |       |          |
| T Chloroethane                     | 0.000                |       | 0      | N.D.                 |       |          |
| T Trichlorofluoromethane           | 0.000                |       | 0      | N.D.                 |       |          |
| T 1,1-Dichloroethene               | 0.000                |       | 0      | N.D.                 |       |          |
| T Methylene chloride               | 3.336                | 49.0  | 1975   | 1.8718               | ng    | m 96     |
| T trans-1,2-Dichloroethene         | 0.000                |       | 0      | N.D.                 |       |          |
| T Methyl tert-butyl ether (MTBE)   | 0.000                |       | 0      | N.D.                 |       |          |
| T 1,1-Dichloroethane               | 0.000                |       | 0      | N.D.                 |       |          |
| T 2,2-Dichloropropane              | 0.000                |       | 0      | N.D.                 |       |          |
| T cis-1,2-Dichloroethene           | 0.000                |       | 0      | N.D.                 |       |          |
| T Methyl ethyl ketone              | 0.000                |       | 0      | N.D.                 |       |          |
| T Bromochloromethane               | 0.000                |       | 0      | N.D.                 |       |          |
| T Chloroform                       | 5.656                | 83.0  | 0      |                      | ng    | md 1     |


# Quantitation Results Report (QT Reviewed)

| Compound                    | RT     | QIon  | Resp. | Conc.   | Units |    | Dev(Min) |
|-----------------------------|--------|-------|-------|---------|-------|----|----------|
| T 1,1,1-Trichloroethane     | 0.000  |       | 0     | N.D.    |       |    |          |
| T Carbon tetrachloride      | 0.000  |       | 0     | N.D.    |       |    |          |
| T 1,1-Dichloropropene       | 0.000  |       | 0     | N.D.    |       |    |          |
| T Benzene                   | 6.278  | 78.0  | 229   | 0.0810  | ng    | m  | 81       |
| T 1,2-Dichloroethane        | 0.000  |       | 0     | N.D.    |       |    |          |
| T Trichloroethene           | 0.000  |       | 0     | N.D.    |       |    |          |
| T 1,2-Dichloropropane       | 0.000  |       | 0     | N.D.    |       |    |          |
| T Dibromomethane            | 0.000  |       | 0     | N.D.    |       |    |          |
| T Bromodichloromethane      | 7.580  | 83.0  | 0     |         | ng    | md | 1        |
| T cis-1,3-Dichloropropene   | 0.000  |       | 0     | N.D.    |       |    |          |
| T Toluene                   | 8.386  | 92.0  | 5263  | 2.9222  | ng    |    | 91       |
| T trans-1,3-Dichloropropene | 0.000  |       | 0     | N.D.    |       |    |          |
| T 1,1,2-Trichloroethane     | 0.000  |       | 0     | N.D.    |       |    |          |
| T Tetrachloroethene         | 0.000  |       | 0     | N.D.    |       |    |          |
| T 1,3-Dichloropropane       | 0.000  |       | 0     | N.D.    |       |    |          |
| T Chlorodibromomethane      | 9.200  | 129.0 | 5690  | 10.1448 | ng    | m  | 97       |
| T 1,2-Dibromoethane         | 0.000  |       | 0     | N.D.    |       |    |          |
| T Chlorobenzene             | 0.000  |       | 0     | N.D.    |       |    |          |
| T 1,1,1,2-Tetrachloroethane | 0.000  |       | 0     | N.D.    |       |    |          |
| T Ethylbenzene              | 0.000  |       | 0     | N.D.    |       |    |          |
| T m+p-Xylenes               | 10.037 | 106.0 | 0     |         | ng    | md | 1        |
| T o-Xylene                  | 0.000  |       | 0     | N.D.    |       |    |          |
| T Styrene                   | 0.000  |       | 0     | N.D.    |       |    |          |
| T Bromoform                 | 10.628 | 172.5 | 2536  | 10.0531 | ng    |    | 95       |
| T Bromobenzene              | 0.000  |       | 0     | N.D.    |       |    |          |
| T 1,1,2,2-Tetrachloroethane | 0.000  |       | 0     | N.D.    |       |    |          |
| T 1,2,3-Trichloropropane    | 0.000  |       | 0     | N.D.    |       |    |          |
| T 2-Chlorotoluene           | 0.000  |       | 0     | N.D.    |       |    |          |
| T 4-Chlorotoluene           | 0.000  |       | 0     | N.D.    |       |    |          |
| T 1,3-Dichlorobenzene       | 0.000  |       | 0     | N.D.    |       |    |          |
| T 1,4-Dichlorobenzene       | 0.000  |       | 0     | N.D.    |       |    |          |
| T 1,2-Dichlorobenzene       | 0.000  |       | 0     | N.D.    |       |    |          |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (\*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

# Quantitation Results Report (QT Reviewed)


| Compound                | Conc. | Exp RT | QIon | Exp Ratio |
|-------------------------|-------|--------|------|-----------|
| Dichlorodifluoromethane | N.D.  | 1.24   | 87.0 | 32.3      |




| Compound      | Conc.  | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------|--------|------|----------|-------|------|--------|-------|-------|
| Chloromethane | 2.0632 | 1.41 | 0.00     | 2332  | 52.0 | 31.5   | 2.1   | 62.1  |



| Compound       | Conc. | Exp RT | QIon | Exp Ratio |
|----------------|-------|--------|------|-----------|
| Vinyl chloride | N.D.  | 1.50   | 64.0 | 29.9      |




| Compound     | Conc. | Exp RT | QIon | Exp Ratio |
|--------------|-------|--------|------|-----------|
| Bromomethane | N.D.  | 1.80   | 94.0 | 104.6     |




# Quantitation Results Report (QT Reviewed)


| Compound     | Conc. | Exp RT | QIon | Exp Ratio |
|--------------|-------|--------|------|-----------|
| Chloroethane | N.D.  | 1.89   | 66.0 | 30.1      |

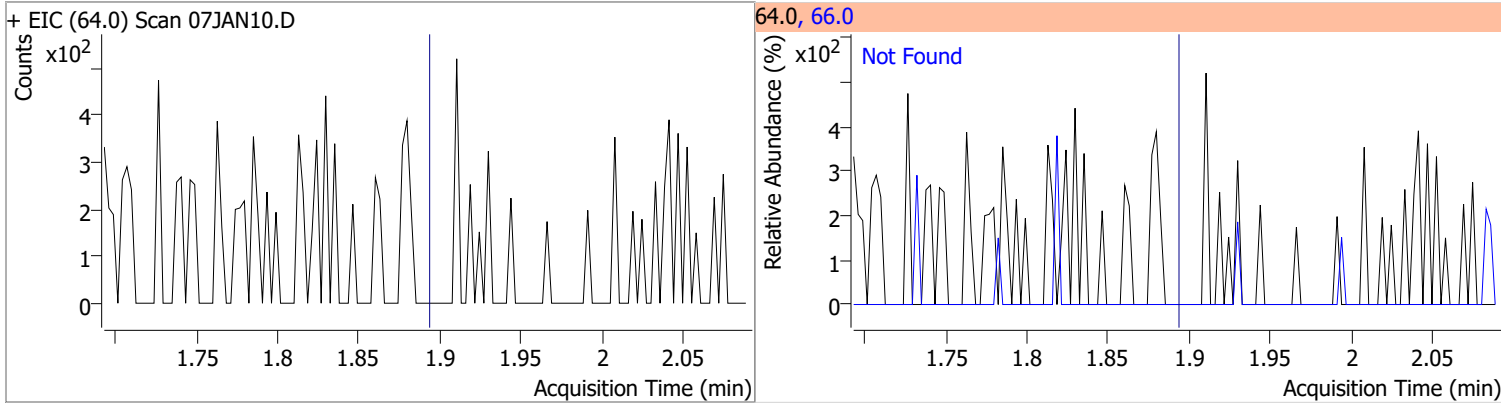


| Compound               | Conc. | Exp RT | QIon  | Exp Ratio |
|------------------------|-------|--------|-------|-----------|
| Trichlorofluoromethane | N.D.  | 2.14   | 103.0 | 64.2      |

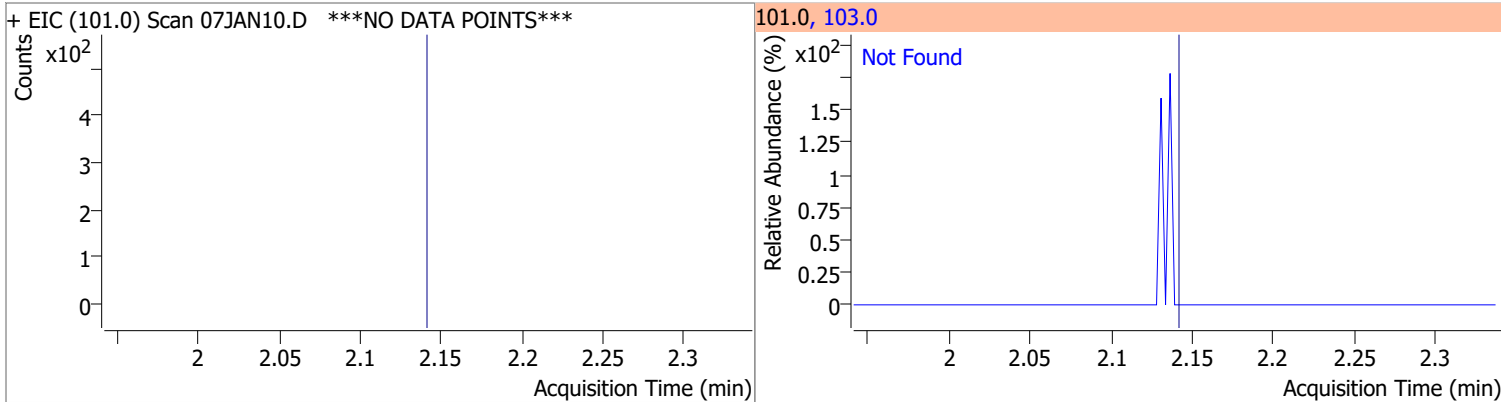

| Compound           | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethene | N.D.  | 2.70   | 61.0 | 180.3     | 63.0 | 56.7      |

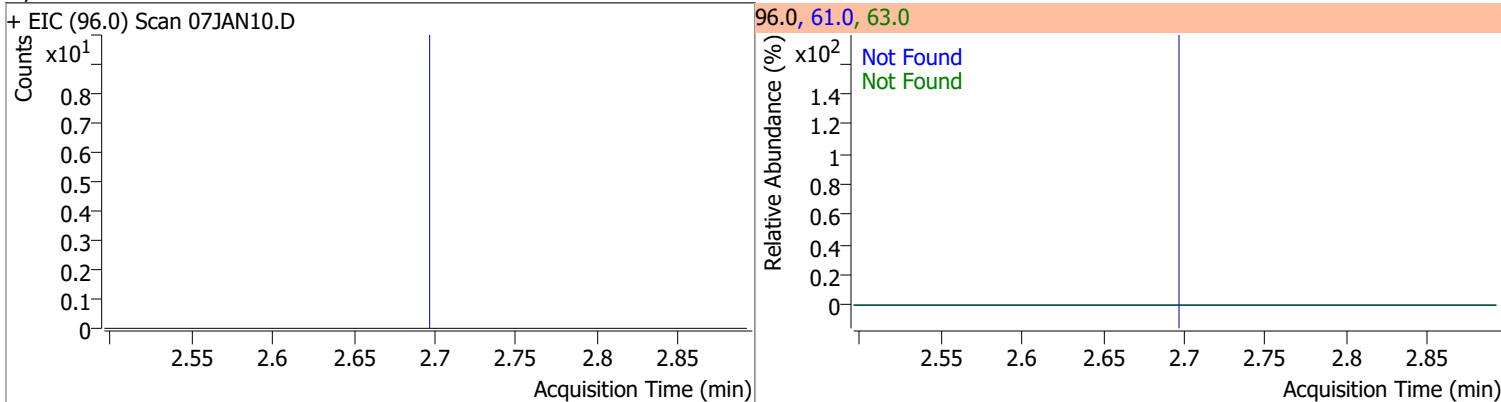


| Compound           | Conc.  | RT   | Dev(Min) | Resp.    | QIon | QRatio | Lower | Upper |
|--------------------|--------|------|----------|----------|------|--------|-------|-------|
| Methylene chloride | 1.8718 | 3.34 | 0.00     | 1975 (m) | 84.0 | 65.3   | 36.9  | 96.9  |
|                    |        |      |          |          | 86.0 | 40.3   | 14.3  | 74.3  |

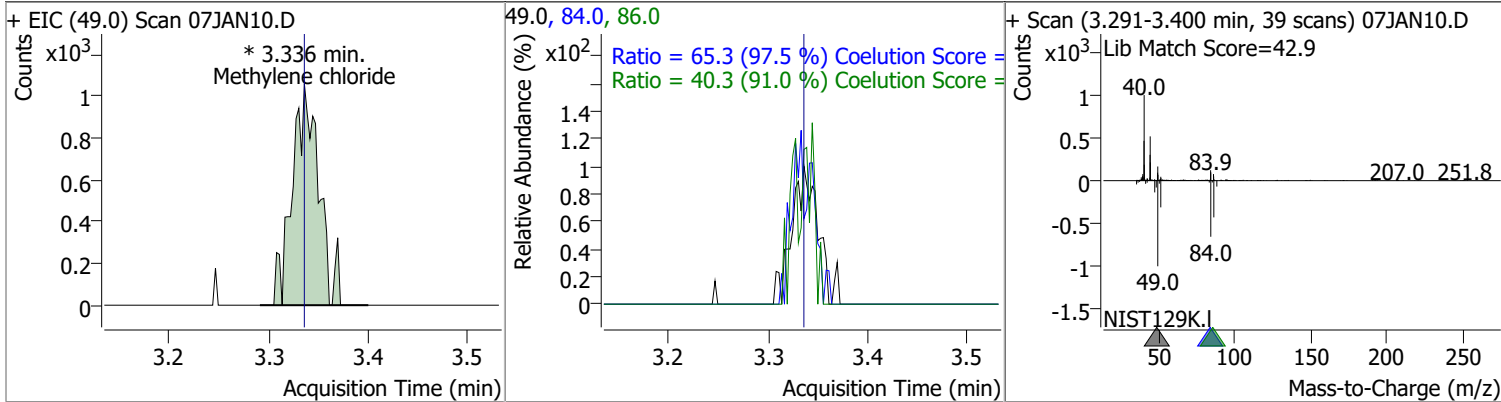




# Quantitation Results Report (QT Reviewed)


| Compound                 | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,2-Dichloroethene | N.D.  | 3.72   | 61.0 | 153.9     | 98.0 | 65.7      |




| Compound                       | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------------------|-------|--------|------|-----------|
| Methyl tert-butyl ether (MTBE) | N.D.  | 3.75   | 57.0 | 24.6      |



| Compound           | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethane | N.D.  | 4.38   | 65.0 | 32.1      | 83.0 | 13.7      |




| Compound            | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|------|-----------|
| 2,2-Dichloropropane | N.D.  | 5.20   | 41.0 | 66.5      | 97.0 | 23.2      |




# Quantitation Results Report (QT Reviewed)


| Compound               | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|------------------------|-------|--------|------|-----------|------|-----------|
| cis-1,2-Dichloroethene | N.D.  | 5.22   | 61.0 | 167.2     | 98.0 | 67.3      |

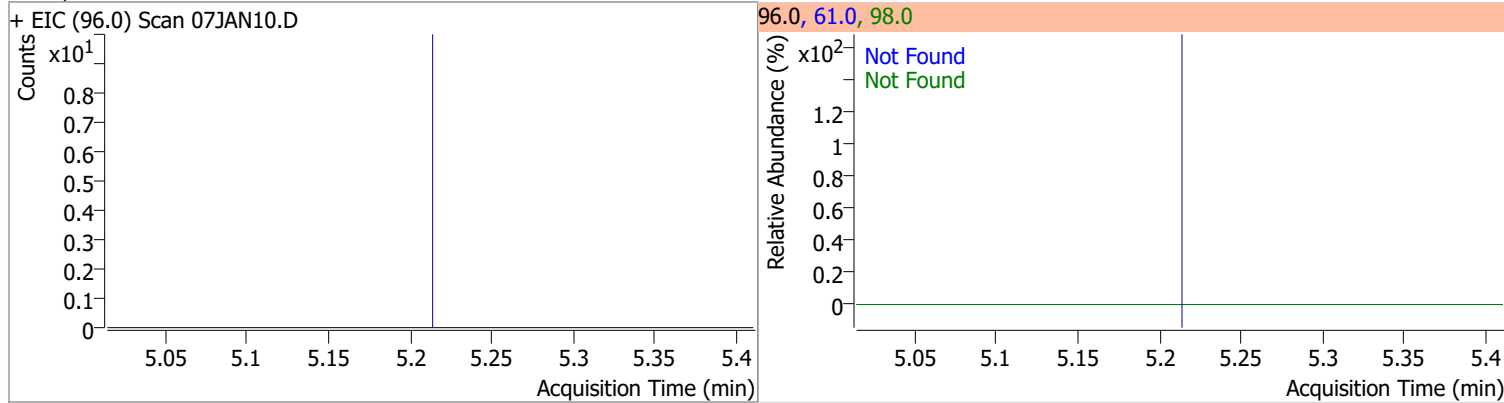


| Compound            | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| Methyl ethyl ketone | N.D.  | 5.28   | 72.0 | 21.3      |

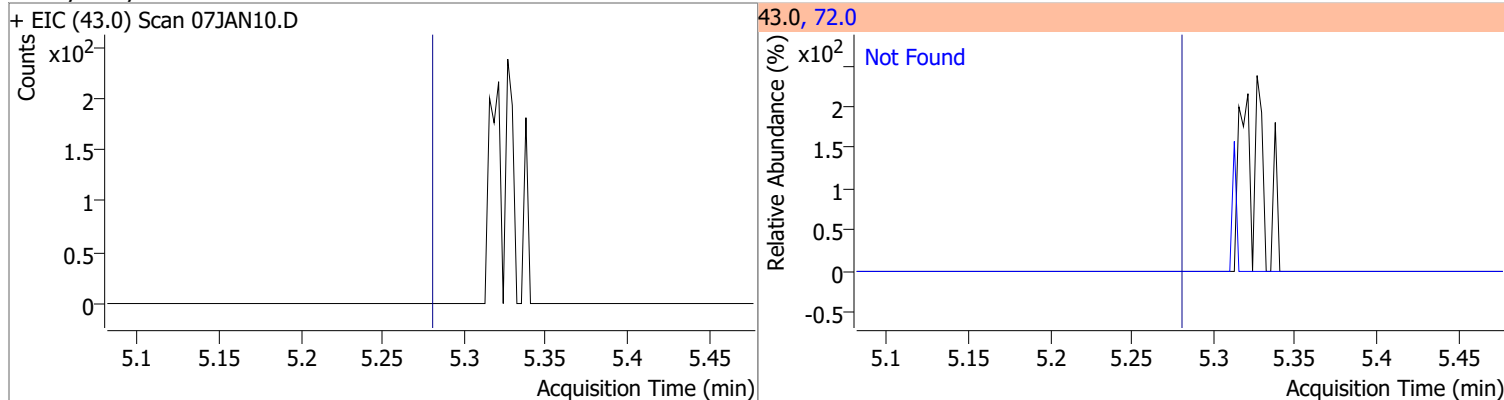

| Compound           | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|
| Bromochloromethane | N.D.  | 5.52   | 49.0 | 182.9     |

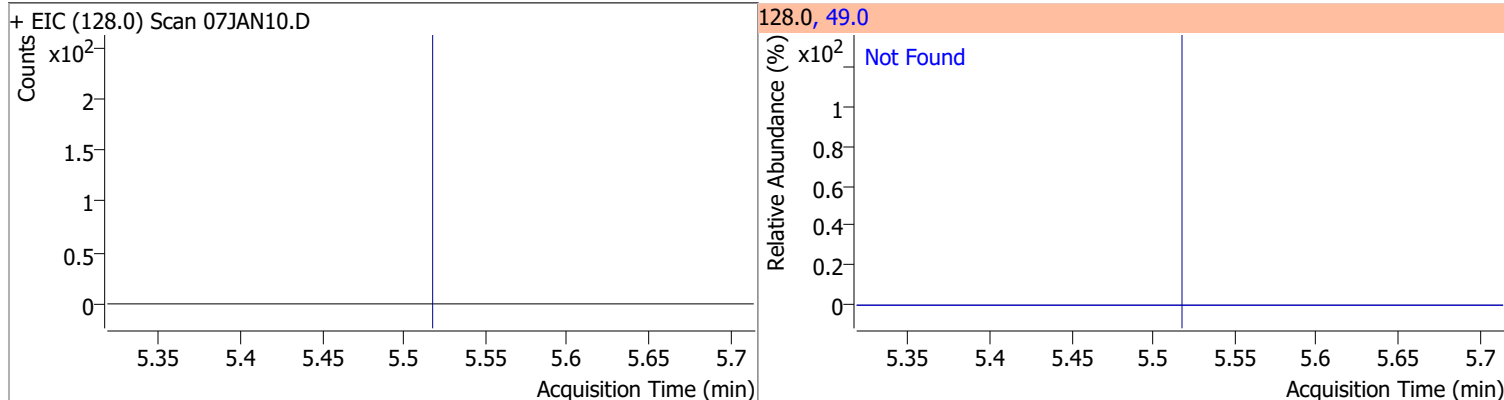


| Compound   | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|------------|-------|----|----------|-------|------|--------|-------|-------|
| Chloroform |       | 0  |          | 0     | 85.0 |        | 36.0  | 96.0  |

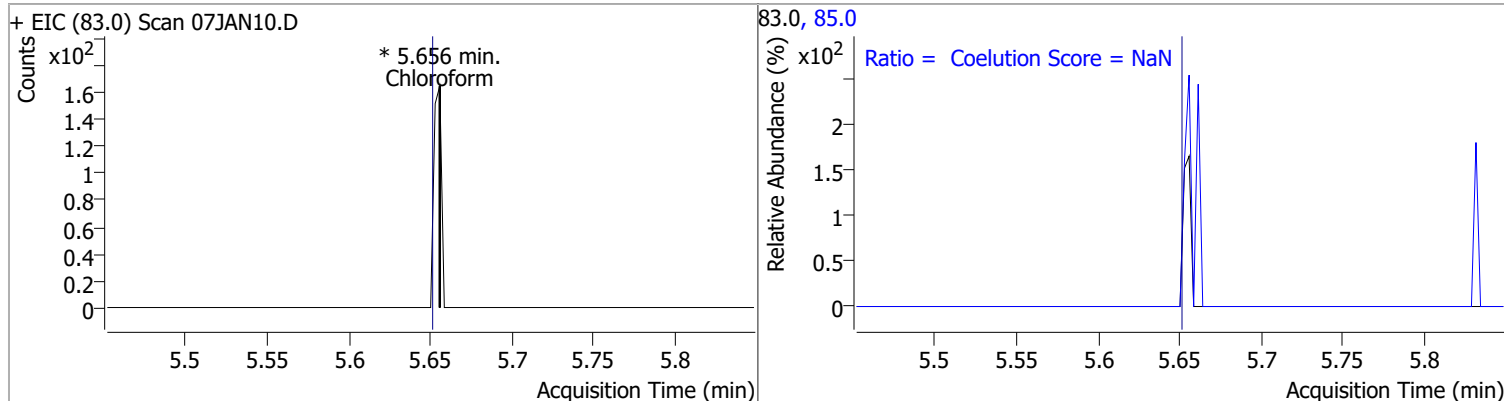


# Quantitation Results Report (QT Reviewed)


| Compound              | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------------|-------|--------|------|-----------|------|-----------|
| 1,1,1-Trichloroethane | N.D.  | 5.83   | 99.0 | 64.7      | 61.0 | 48.1      |




| Compound             | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Dibromofluoromethane | 283.6314 | 5.85 | 0.00     | 189885 | 191.5 | 22.4   | 0.0   | 53.1  |



| Compound             | Conc. | Exp RT | QIon  | Exp Ratio | QIon  | Exp Ratio |
|----------------------|-------|--------|-------|-----------|-------|-----------|
| Carbon tetrachloride | N.D.  | 6.02   | 119.0 | 97.2      | 121.0 | 30.1      |

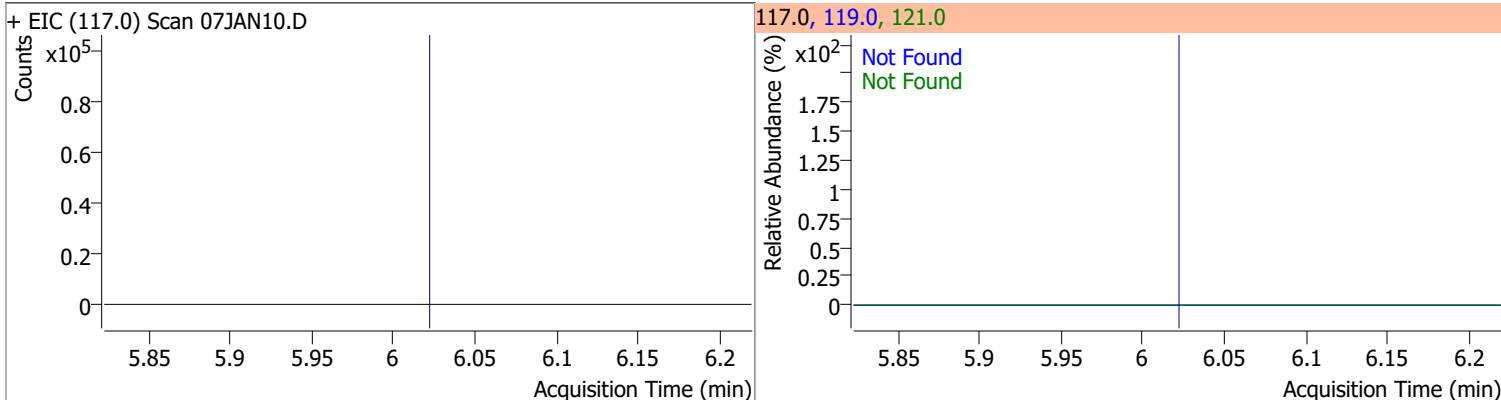


| Compound            | Conc. | Exp RT | QIon  | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|-------|-----------|------|-----------|
| 1,1-Dichloropropene | N.D.  | 6.04   | 110.0 | 35.9      | 77.0 | 30.1      |

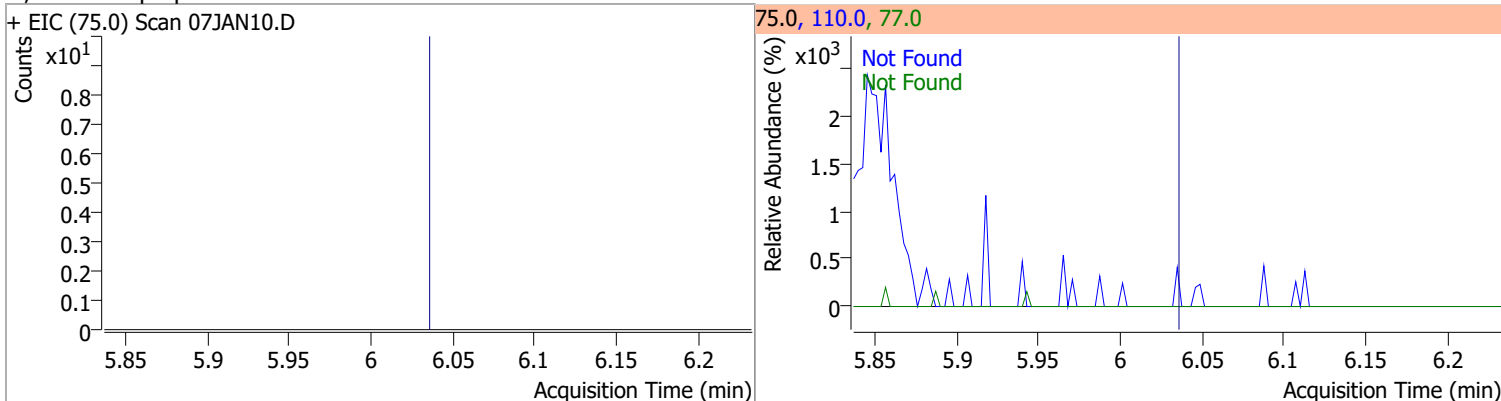


# Quantitation Results Report (QT Reviewed)


| Compound              | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 305.1186 | 6.23 | 0.00     | 88230 | 65.0 | 194.6  | 166.5 | 226.5 |




| Compound | Conc.  | RT   | Dev(Min) | Resp.   | QIon | QRatio | Lower | Upper |
|----------|--------|------|----------|---------|------|--------|-------|-------|
| Benzene  | 0.0810 | 6.28 | 0.00     | 229 (m) | 77.0 | 14.2   | 0.0   | 53.5  |

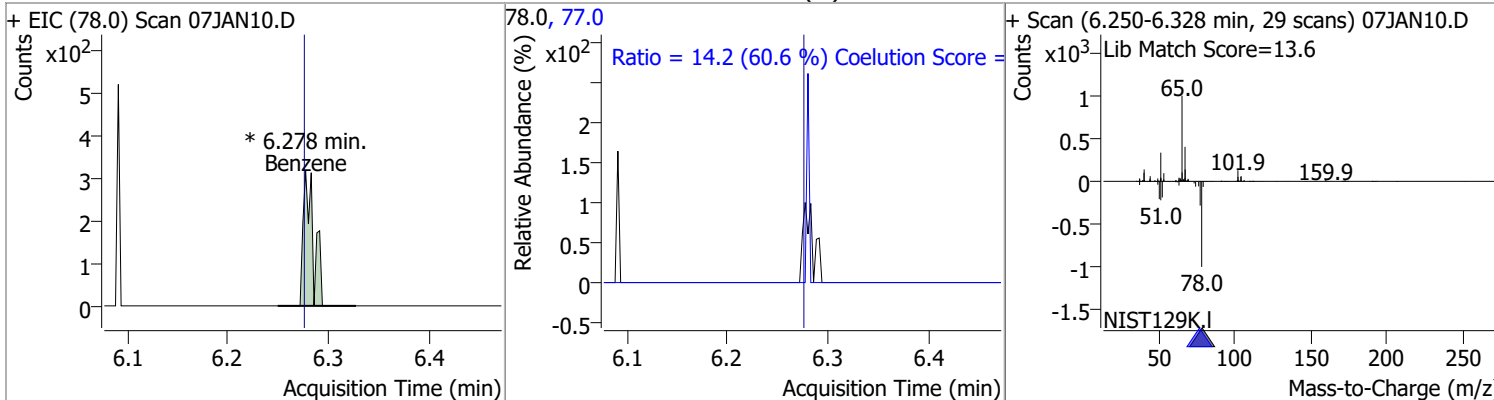





| Compound           | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,2-Dichloroethane | N.D.  | 6.32   | 64.0 | 29.9      | 98.0 | 7.6       |



| Compound        | Conc. | Exp RT | QIon  | Exp Ratio | QIon | Exp Ratio |
|-----------------|-------|--------|-------|-----------|------|-----------|
| Trichloroethene | N.D.  | 7.03   | 130.0 | 101.5     | 97.0 | 64.1      |




# Quantitation Results Report (QT Reviewed)

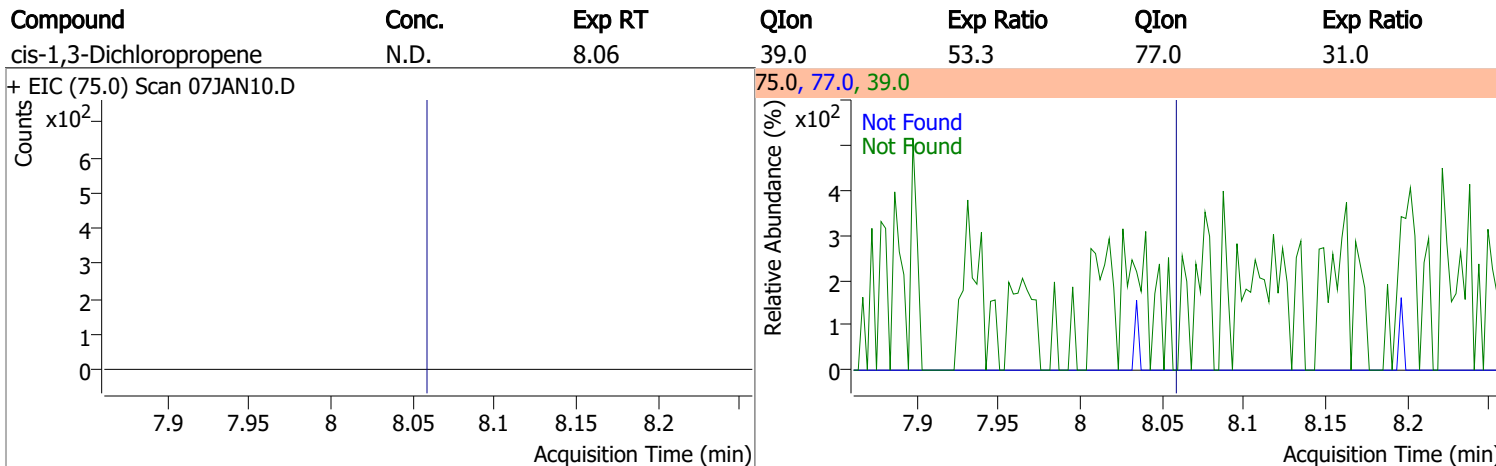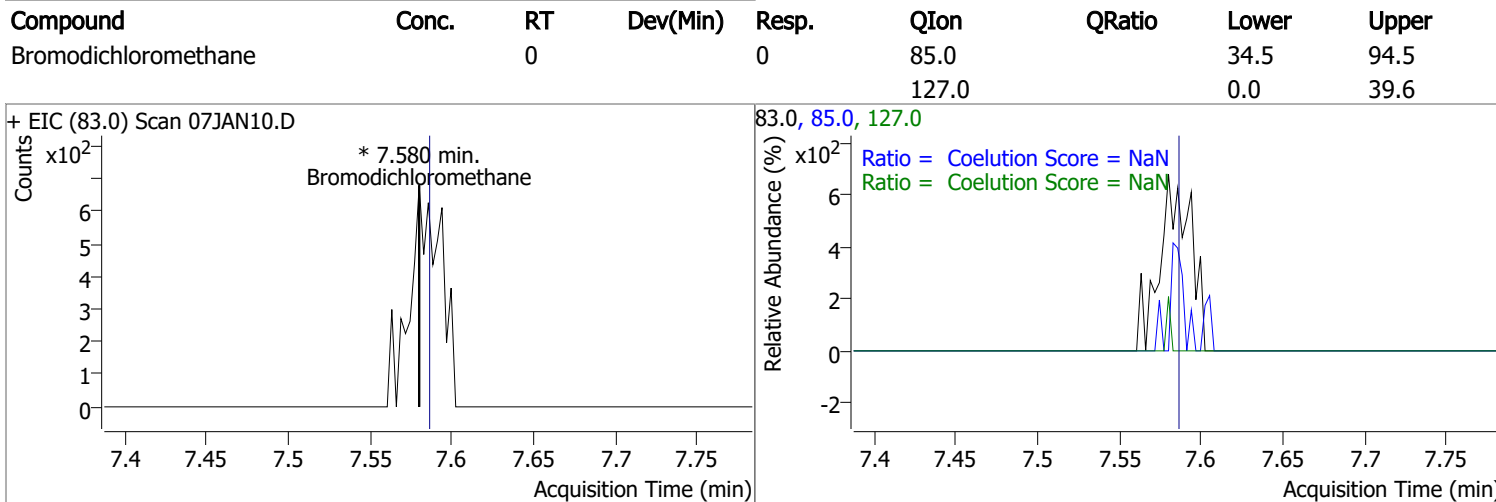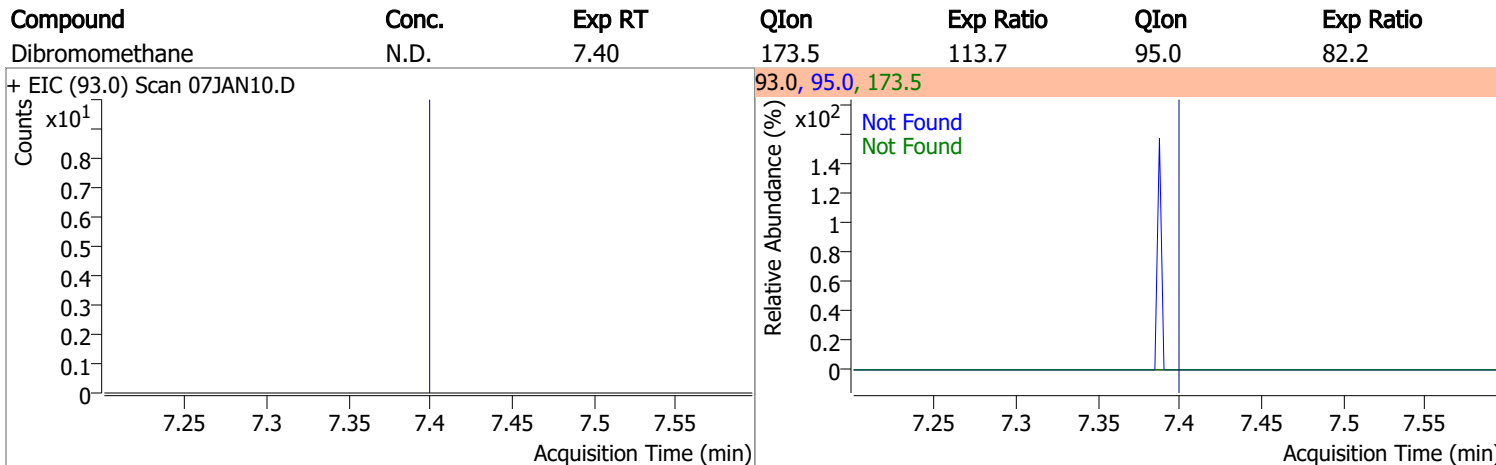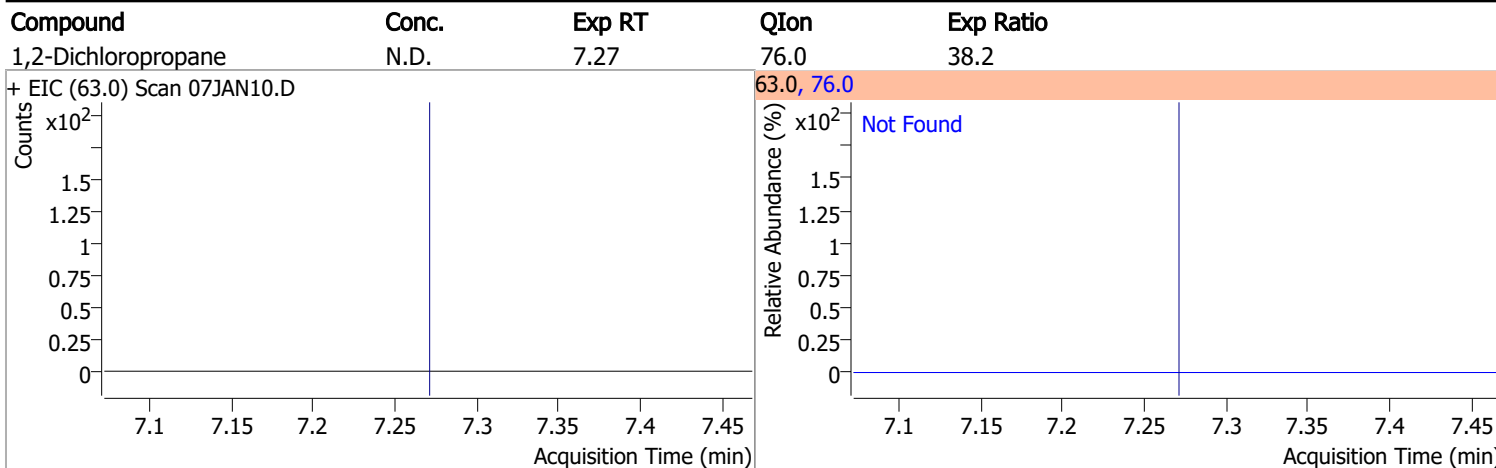


# Quantitation Results Report (QT Reviewed)


| Compound   | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 262.5368 | 8.32 | 0.00     | 699981 | 100.0 | 65.4   | 34.4  | 94.4  |
|            |          |      |          |        | 99.0  | 9.7    | 0.0   | 39.6  |

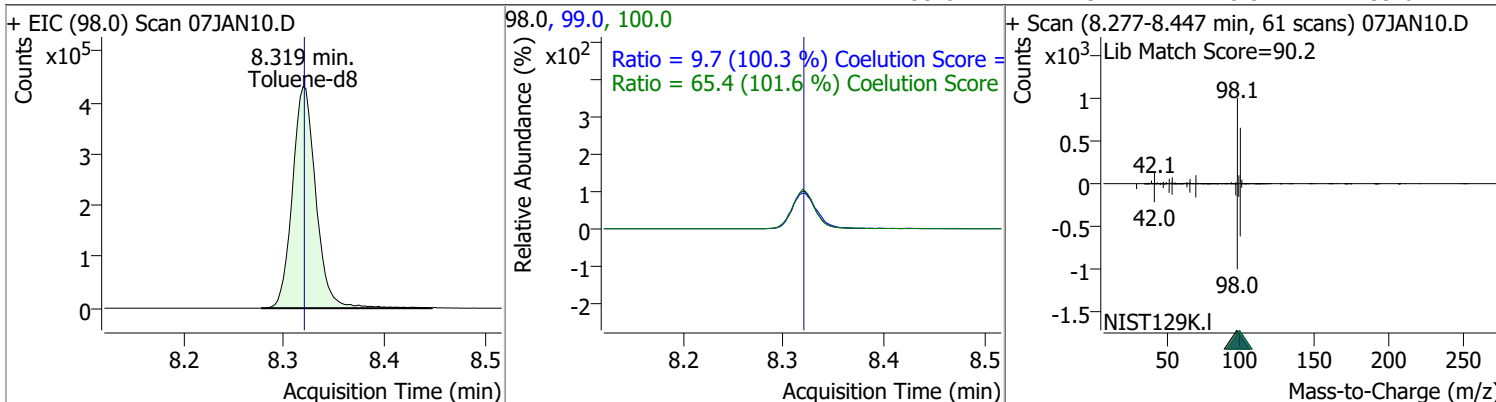


| Compound | Conc.  | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|--------|------|----------|-------|------|--------|-------|-------|
| Toluene  | 2.9222 | 8.39 | 0.00     | 5263  | 91.0 | 187.9  | 145.8 | 205.8 |

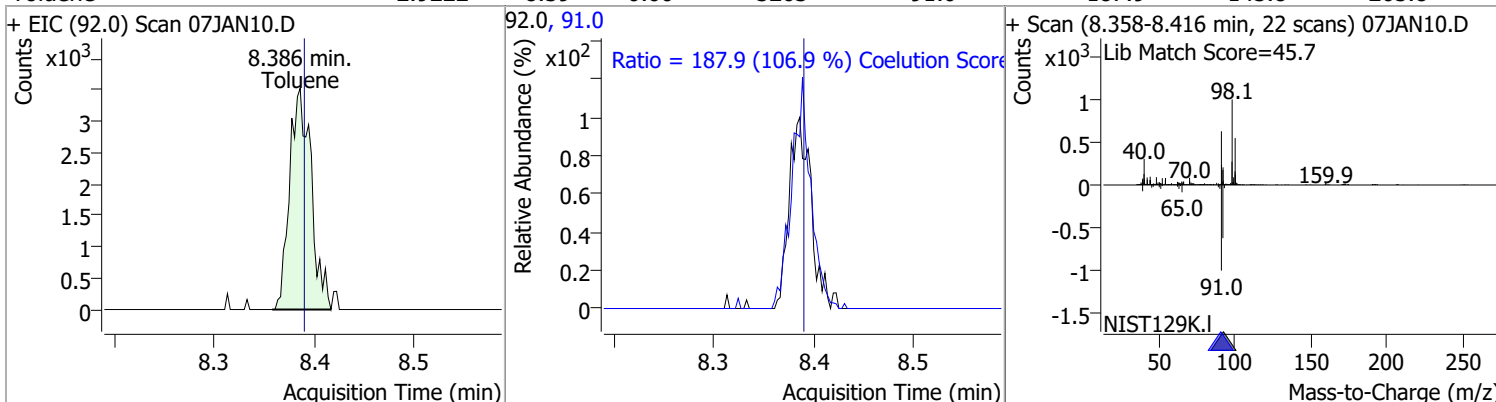

| Compound                  | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,3-Dichloropropene | N.D.  | 8.64   | 39.0 | 53.4      | 77.0 | 32.4      |

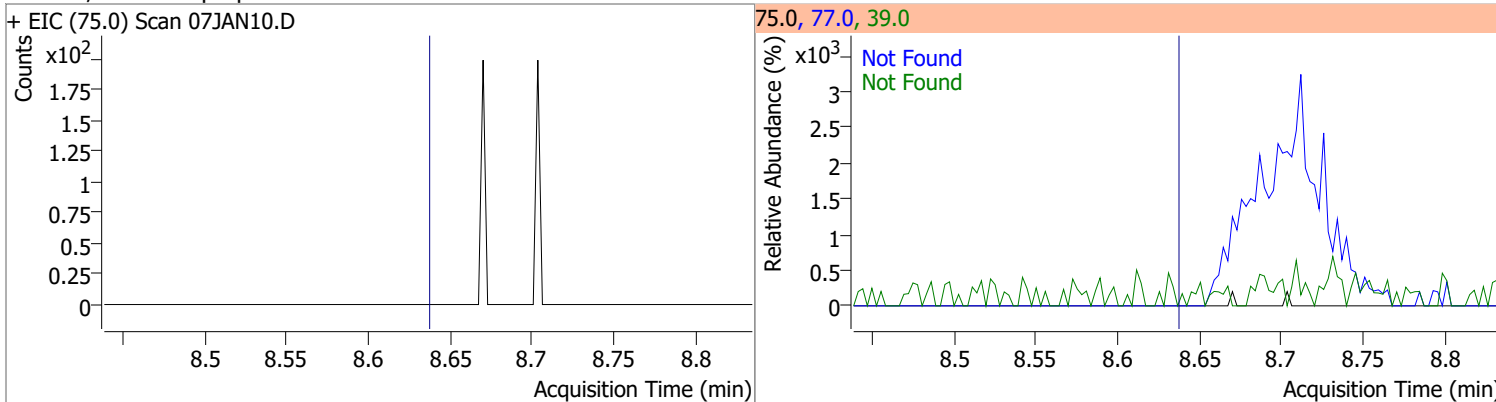


| Compound              | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------------|-------|--------|------|-----------|------|-----------|
| 1,1,2-Trichloroethane | N.D.  | 8.82   | 97.0 | 114.6     | 85.0 | 67.6      |

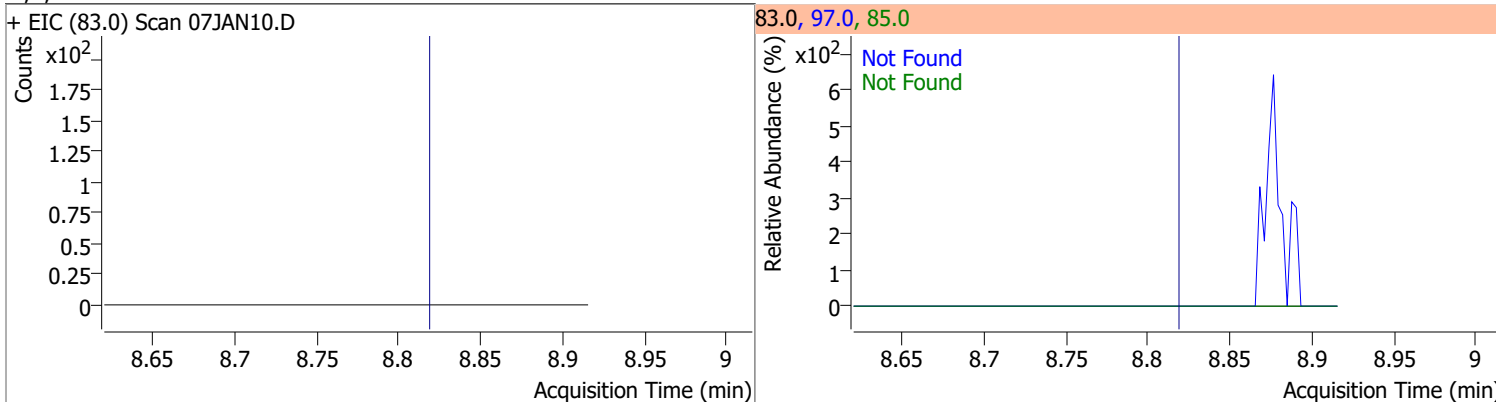


# Quantitation Results Report (QT Reviewed)


| Compound          | Conc. | Exp RT | QIon  | Exp Ratio | QIon  | Exp Ratio |
|-------------------|-------|--------|-------|-----------|-------|-----------|
| Tetrachloroethene | N.D.  | 8.94   | 165.8 | 128.6     | 129.0 | 91.5      |




| Compound            | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| 1,3-Dichloropropane | N.D.  | 8.98   | 78.0 | 32.9      |



| Compound             | Conc.   | RT   | Dev(Min) | Resp.    | QIon  | QRatio | Lower | Upper |
|----------------------|---------|------|----------|----------|-------|--------|-------|-------|
| Chlorodibromomethane | 10.1448 | 9.20 | -0.01    | 5690 (m) | 127.0 | 80.7   | 48.0  | 108.0 |




| Compound          | Conc. | Exp RT | QIon  | Exp Ratio |
|-------------------|-------|--------|-------|-----------|
| 1,2-Dibromoethane | N.D.  | 9.31   | 109.0 | 94.5      |




# Quantitation Results Report (QT Reviewed)


| Compound      | Conc. | Exp RT | QIon  | Exp Ratio |
|---------------|-------|--------|-------|-----------|
| Chlorobenzene | N.D.  | 9.80   | 114.0 | 32.1      |

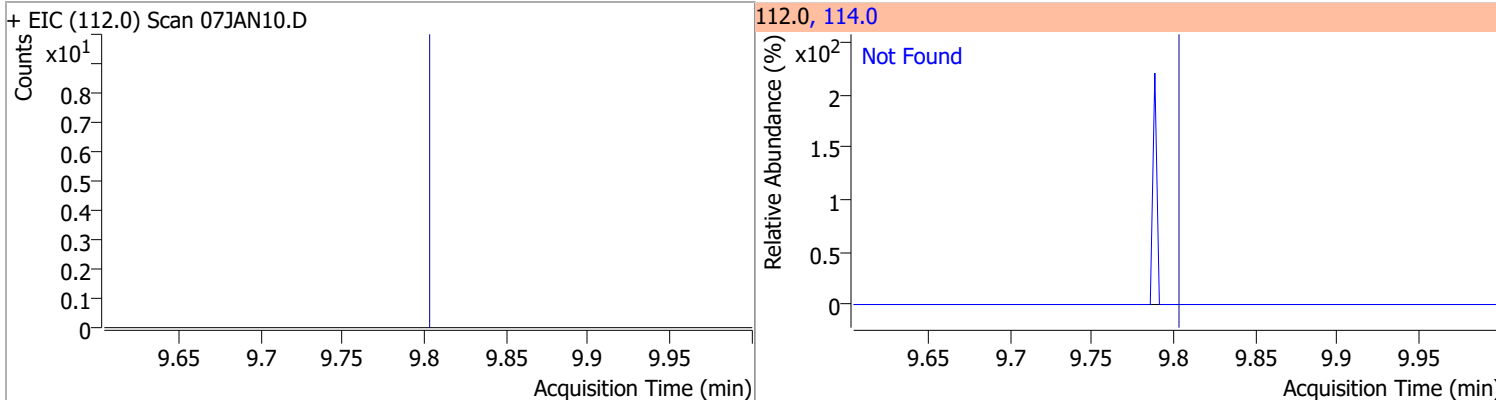


| Compound                  | Conc. | Exp RT | QIon  | Exp Ratio |
|---------------------------|-------|--------|-------|-----------|
| 1,1,1,2-Tetrachloroethane | N.D.  | 9.89   | 133.0 | 98.6      |

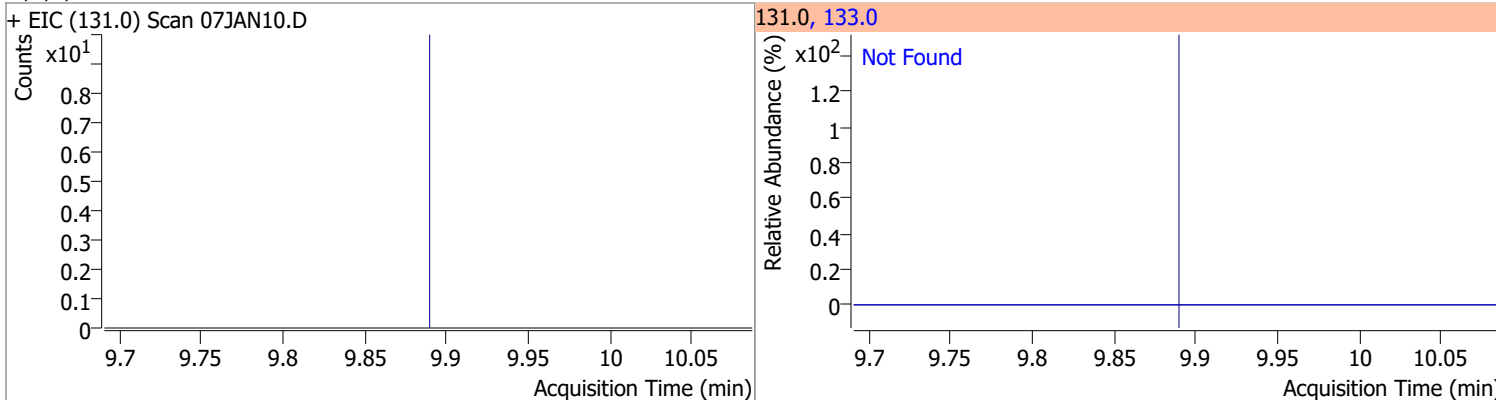

| Compound     | Conc. | Exp RT | QIon  | Exp Ratio |
|--------------|-------|--------|-------|-----------|
| Ethylbenzene | N.D.  | 9.92   | 106.0 | 31.1      |




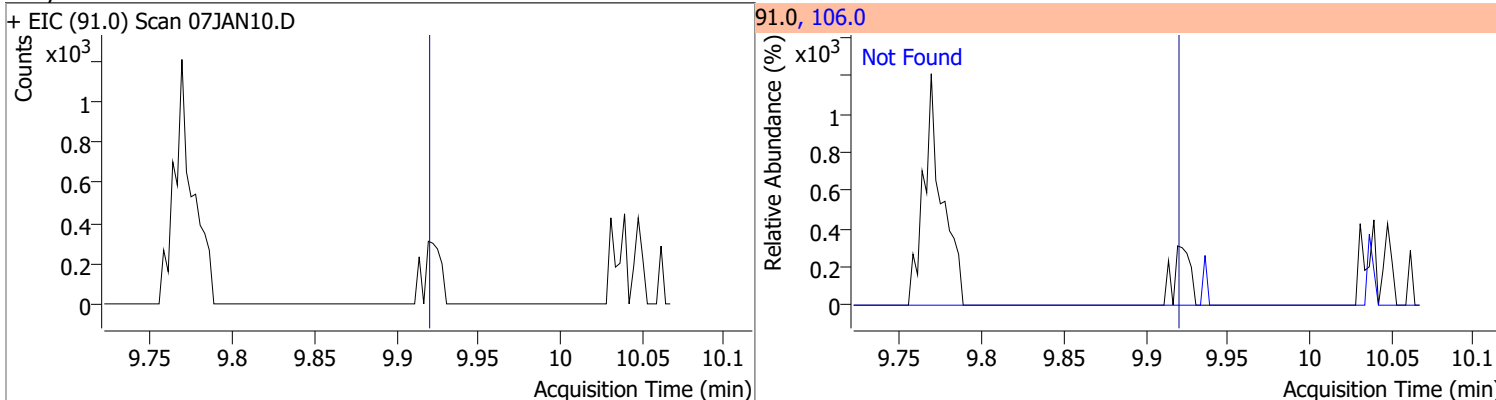


| Compound    | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-------------|-------|----|----------|-------|------|--------|-------|-------|
| m+p-Xylenes |       | 0  |          | 0     | 91.0 |        | 171.4 | 231.4 |

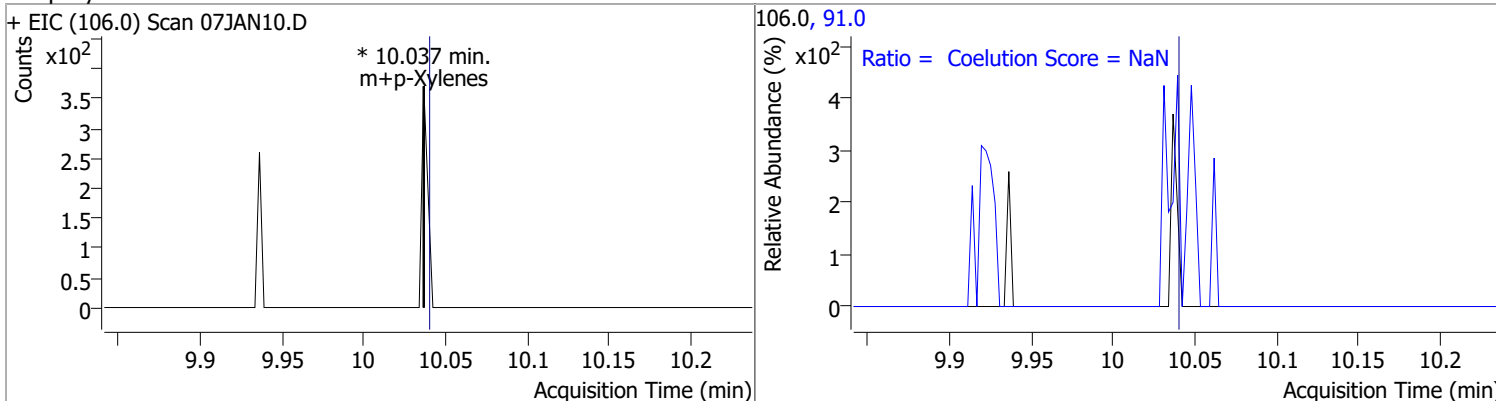











# Quantitation Results Report (QT Reviewed)



# Quantitation Results Report (QT Reviewed)


| Compound                                          | Conc. | Exp RT | QIon               | Exp Ratio | QIon  | Exp Ratio |
|---------------------------------------------------|-------|--------|--------------------|-----------|-------|-----------|
| Bromobenzene                                      | N.D.  | 11.09  | 77.0               | 145.7     | 158.0 | 96.5      |
| + EIC (156.0) Scan 07JAN10.D ***NO DATA POINTS*** |       |        | 156.0, 77.0, 158.0 |           |       |           |
|                                                   |       |        |                    |           |       |           |
| 1,1,2,2-Tetrachloroethane                         | N.D.  | 11.12  | 85.0               | 66.2      |       |           |
| + EIC (83.0) Scan 07JAN10.D                       |       |        | 83.0, 85.0         |           |       |           |
|                                                   |       |        |                    |           |       |           |
| 1,2,3-Trichloropropane                            | N.D.  | 11.15  | 112.0              | 63.5      |       |           |
| + EIC (110.0) Scan 07JAN10.D                      |       |        | 110.0, 112.0       |           |       |           |
|                                                   |       |        |                    |           |       |           |
| 2-Chlorotoluene                                   | N.D.  | 11.29  | 91.0               | 282.3     |       |           |
| + EIC (126.0) Scan 07JAN10.D ***NO DATA POINTS*** |       |        | 126.0, 91.0        |           |       |           |
|                                                   |       |        |                    |           |       |           |

# Quantitation Results Report (QT Reviewed)
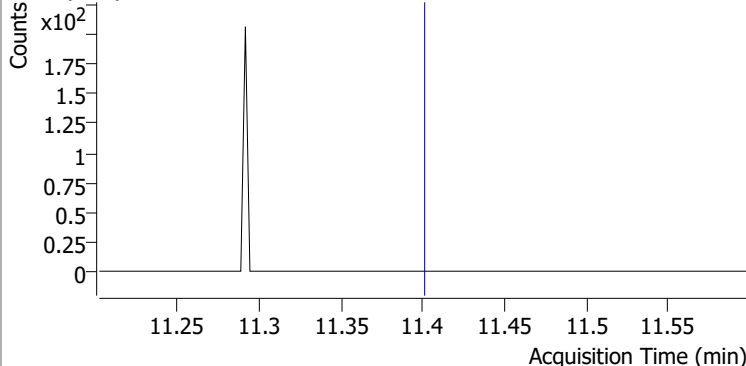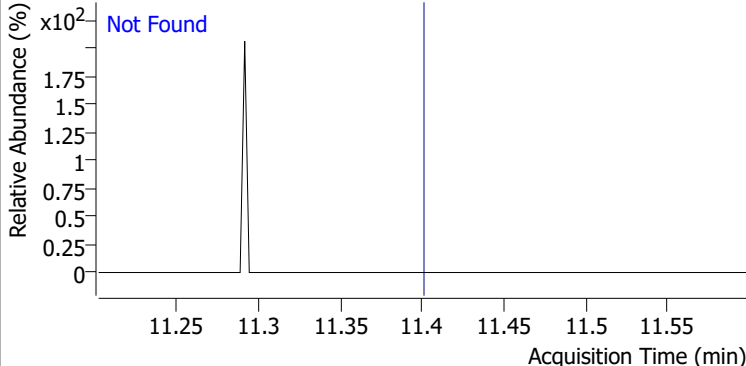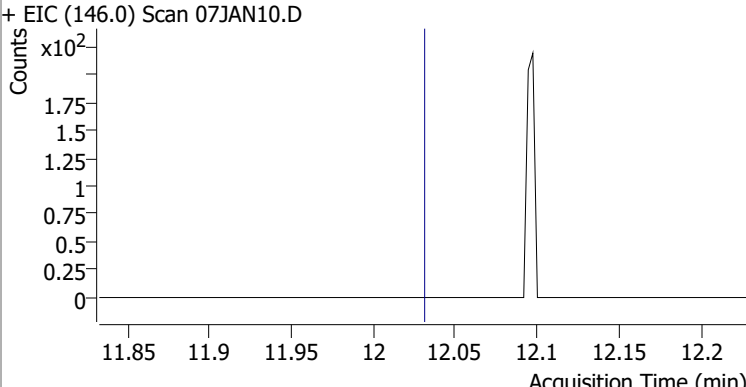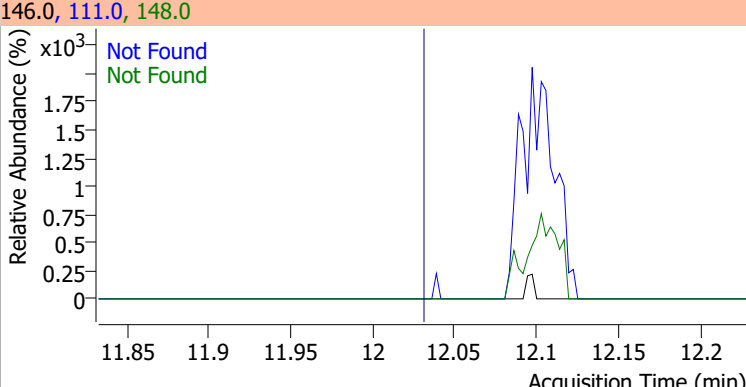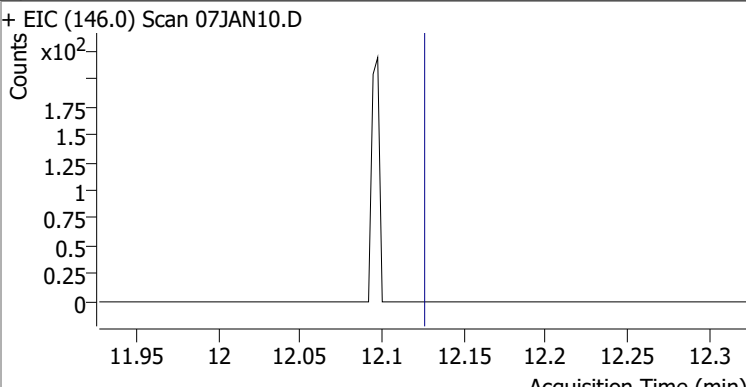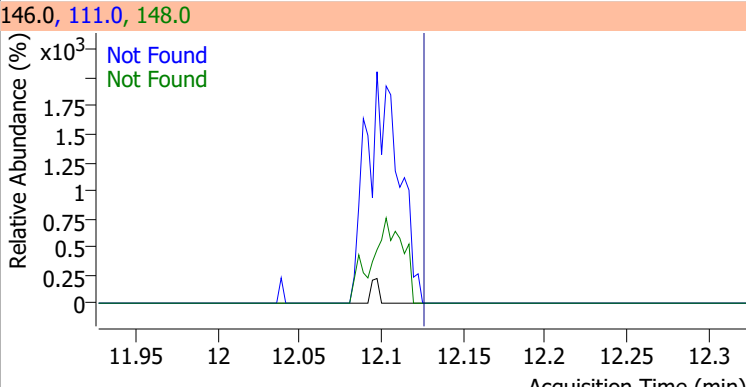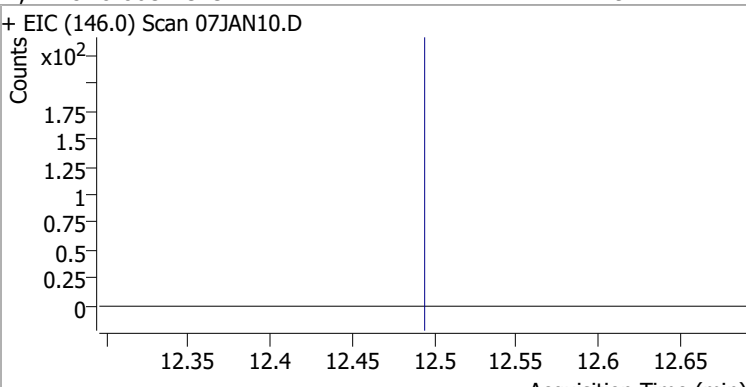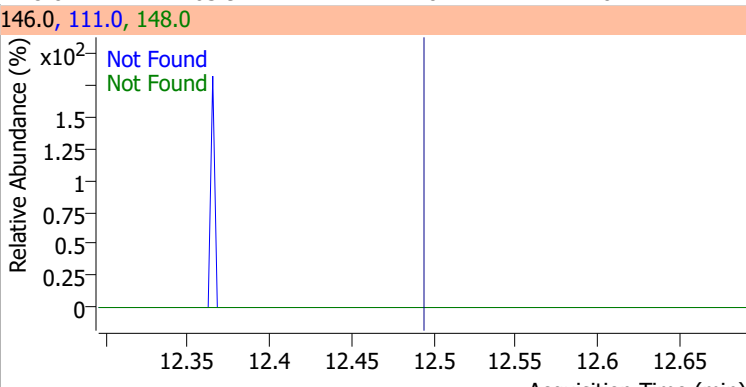
| Compound                                                                           | Conc. | Exp RT | QIon                                                                                 | Exp Ratio |      |           |
|------------------------------------------------------------------------------------|-------|--------|--------------------------------------------------------------------------------------|-----------|------|-----------|
| 4-Chlorotoluene                                                                    | N.D.  | 11.40  | 126.0                                                                                | 31.7      |      |           |
| + EIC (91.0) Scan 07JAN10.D                                                        |       |        | 91.0, 126.0                                                                          |           |      |           |
|    |       |        |    |           |      |           |
| 1,3-Dichlorobenzene                                                                | N.D.  | 12.03  | 148.0                                                                                | 63.6      | QIon | Exp Ratio |
| + EIC (146.0) Scan 07JAN10.D                                                       |       |        | 146.0, 111.0, 148.0                                                                  |           |      |           |
|   |       |        |   |           |      |           |
| 1,4-Dichlorobenzene                                                                | N.D.  | 12.13  | 148.0                                                                                | 63.1      | QIon | Exp Ratio |
| + EIC (146.0) Scan 07JAN10.D                                                       |       |        | 146.0, 111.0, 148.0                                                                  |           |      |           |
|  |       |        |  |           |      |           |
| 1,2-Dichlorobenzene                                                                | N.D.  | 12.49  | 148.0                                                                                | 63.9      | QIon | Exp Ratio |
| + EIC (146.0) Scan 07JAN10.D                                                       |       |        | 146.0, 111.0, 148.0                                                                  |           |      |           |
|  |       |        |  |           |      |           |

# Quantitation Results Report (QT Reviewed)

|                |                                     |                   |                       |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File      | 07JAN11.D                           | Operator          | MSC                   |
| Acq. Method    | 5975CACQF.M                         | Acq. Date-Time    | 1/7/2022 2:14:04 PM   |
| Sample Name    | B22010219-001F                      | Instrument        | VOA5975C              |
| Vial           | 11                                  | Multiplier        | 1.00                  |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m  | Comment           |                       |
| Tune File      | BFB_Atune3.u                        | Tune Date         | 10/11/2021 4:02:00 PM |
| Batch Name     | VG010722_8260B.batch.bin            | Last Calib Update | 3/2/2022 10:41:44 AM  |
| Ref Library    | \\MASSHUNTER\Org\Library\NIST129K.l |                   |                       |







| Compound                           | RT                   | QIon  | Resp.  | Conc.                | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|----------------------|-------|----------|
| <b>Internal Standards</b>          |                      |       |        |                      |       |          |
| M Fluorobenzene                    | 6.621                | 96.0  | 806641 | 250.0000             | ng    | -0.003   |
| M Chlorobenzene-d5                 | 9.772                | 82.0  | 312339 | 250.0000             | ng    | 0.000    |
| M 1,4-Dichlorobenzene-d4           | 12.100               | 152.0 | 239572 | 250.0000             | ng    | 0.000    |
| <b>System Monitoring Compounds</b> |                      |       |        |                      |       |          |
| S Dibromofluoromethane             | 5.848                | 113.0 | 211143 | 277.8425             | ng    | 0.003    |
| Spiked Amount: 250.000             | Range: 80.0 - 119.0% |       |        | Recovery = 111.14%   |       |          |
| S 1,2-Dichloroethane-d4            | 6.233                | 67.0  | 96836  | 295.0174             | ng    | 0.000    |
| Spiked Amount: 250.000             | Range: 81.0 - 118.0% |       |        | Recovery = 118.01% * |       |          |
| S Toluene-d8                       | 8.319                | 98.0  | 811840 | 269.7270             | ng    | 0.000    |
| Spiked Amount: 250.000             | Range: 89.0 - 112.0% |       |        | Recovery = 107.89%   |       |          |
| S p-Bromofluorobenzene             | 10.951               | 95.0  | 237586 | 270.6993             | ng    | -0.003   |
| Spiked Amount: 250.000             | Range: 85.0 - 114.0% |       |        | Recovery = 108.28%   |       |          |
| <b>Target Compounds</b>            |                      |       |        |                      |       |          |
| T Dichlorodifluoromethane          | 0.000                |       | 0      | N.D.                 |       |          |
| T Chloromethane                    | 1.417                | 50.0  | 1302   | 1.0151               | ng    | m 84     |
| T Vinyl chloride                   | 0.000                |       | 0      | N.D.                 |       |          |
| T Bromomethane                     | 0.000                |       | 0      | N.D.                 |       |          |
| T Chloroethane                     | 1.899                | 64.0  | 1604   | 2.8067               | ng    | m 94     |
| T Trichlorofluoromethane           | 0.000                |       | 0      | N.D.                 |       |          |
| T 1,1-Dichloroethene               | 0.000                |       | 0      | N.D.                 |       |          |
| T Methylene chloride               | 3.333                | 49.0  | 1285   | 1.0727               | ng    | m 83     |
| T trans-1,2-Dichloroethene         | 0.000                |       | 0      | N.D.                 |       |          |
| T Methyl tert-butyl ether (MTBE)   | 0.000                |       | 0      | N.D.                 |       |          |
| T 1,1-Dichloroethane               | 4.381                | 63.0  | 953    | 0.6175               | ng    | m 76     |
| T 2,2-Dichloropropane              | 0.000                |       | 0      | N.D.                 |       |          |
| T cis-1,2-Dichloroethene           | 0.000                |       | 0      | N.D.                 |       |          |
| T Methyl ethyl ketone              | 0.000                |       | 0      | N.D.                 |       |          |
| T Bromochloromethane               | 0.000                |       | 0      | N.D.                 |       |          |
| T Chloroform                       | 5.650                | 83.0  | 777    | 0.5057               | ng    | m 77     |

# Quantitation Results Report (QT Reviewed)

| Compound                    | RT     | QIon  | Resp. | Conc.  | Units |    | Dev(Min) |
|-----------------------------|--------|-------|-------|--------|-------|----|----------|
| T 1,1,1-Trichloroethane     | 0.000  |       | 0     | N.D.   |       |    |          |
| T Carbon tetrachloride      | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,1-Dichloropropene       | 0.000  |       | 0     | N.D.   |       |    |          |
| T Benzene                   | 6.278  | 78.0  | 1404  | 0.4371 | ng    | m  | 75       |
| T 1,2-Dichloroethane        | 0.000  |       | 0     | N.D.   |       |    |          |
| T Trichloroethene           | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,2-Dichloropropane       | 0.000  |       | 0     | N.D.   |       |    |          |
| T Dibromomethane            | 0.000  |       | 0     | N.D.   |       |    |          |
| T Bromodichloromethane      | 0.000  |       | 0     | N.D.   |       |    |          |
| T cis-1,3-Dichloropropene   | 0.000  |       | 0     | N.D.   |       |    |          |
| T Toluene                   | 8.397  | 92.0  | 699   | 0.3436 | ng    | m  | 84       |
| T trans-1,3-Dichloropropene | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,1,2-Trichloroethane     | 8.812  | 83.0  | 0     |        | ng    | md | 1        |
| T Tetrachloroethene         | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,3-Dichloropropane       | 8.977  | 76.0  | 319   | 0.4005 | ng    | m  | 81       |
| T Chlorodibromomethane      | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,2-Dibromoethane         | 0.000  |       | 0     | N.D.   |       |    |          |
| T Chlorobenzene             | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,1,1,2-Tetrachloroethane | 0.000  |       | 0     | N.D.   |       |    |          |
| T Ethylbenzene              | 0.000  |       | 0     | N.D.   |       |    |          |
| T m+p-Xylenes               | 10.039 | 106.0 | 0     |        | ng    | md | 1        |
| T o-Xylene                  | 10.430 | 106.0 | 0     |        | ng    | md | 1        |
| T Styrene                   | 0.000  |       | 0     | N.D.   |       |    |          |
| T Bromoform                 | 0.000  |       | 0     | N.D.   |       |    |          |
| T Bromobenzene              | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,1,2,2-Tetrachloroethane | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,2,3-Trichloropropane    | 0.000  |       | 0     | N.D.   |       |    |          |
| T 2-Chlorotoluene           | 0.000  |       | 0     | N.D.   |       |    |          |
| T 4-Chlorotoluene           | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,3-Dichlorobenzene       | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,4-Dichlorobenzene       | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,2-Dichlorobenzene       | 0.000  |       | 0     | N.D.   |       |    |          |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (\*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

# Quantitation Results Report (QT Reviewed)

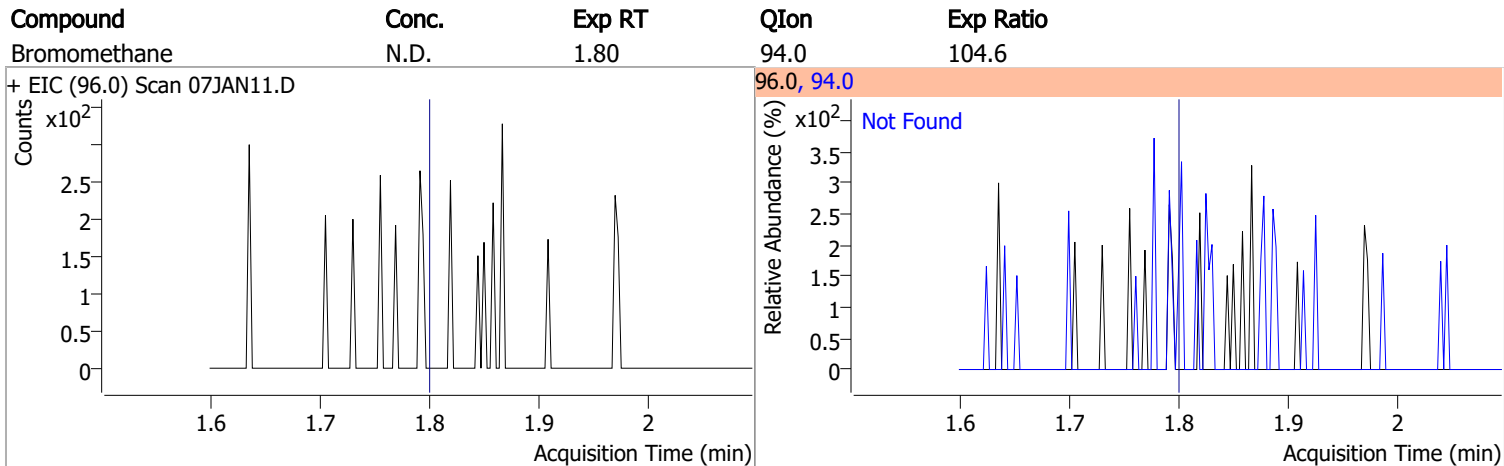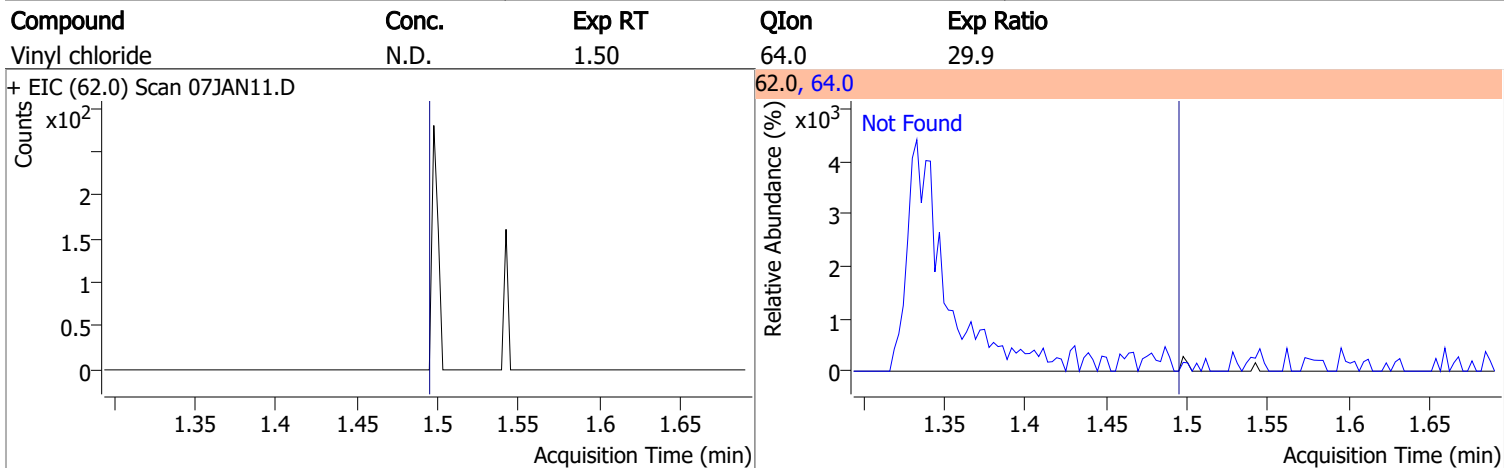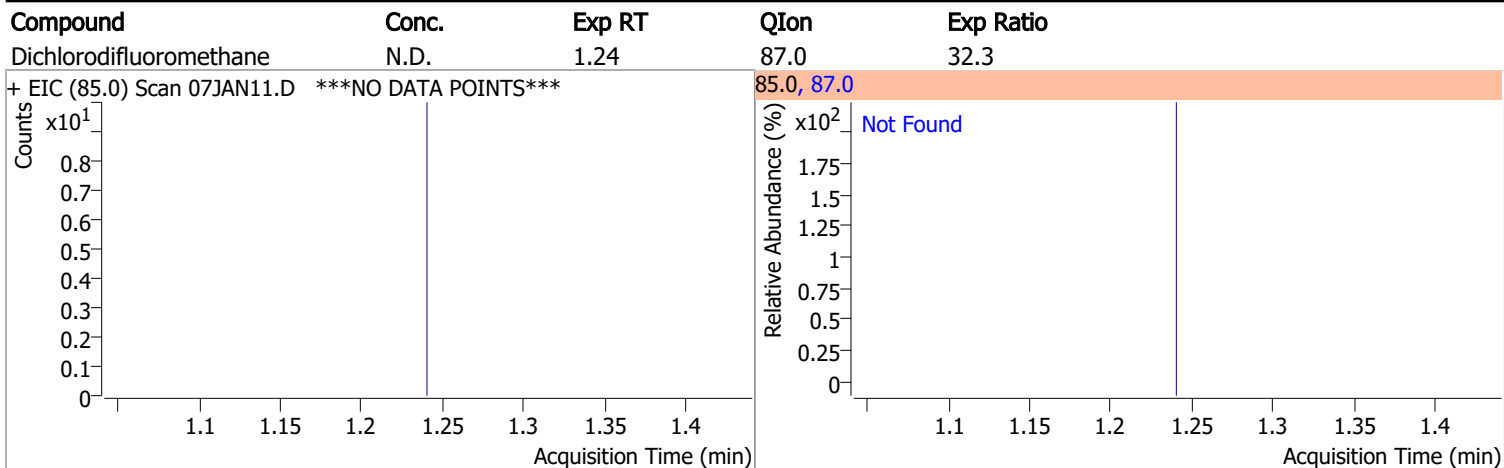


# Quantitation Results Report (QT Reviewed)


| Compound     | Conc.  | RT   | Dev(Min) | Resp.    | QIon | QRatio | Lower | Upper |
|--------------|--------|------|----------|----------|------|--------|-------|-------|
| Chloroethane | 2.8067 | 1.90 | 0.01     | 1604 (m) | 66.0 | 27.0   | 0.1   | 60.1  |

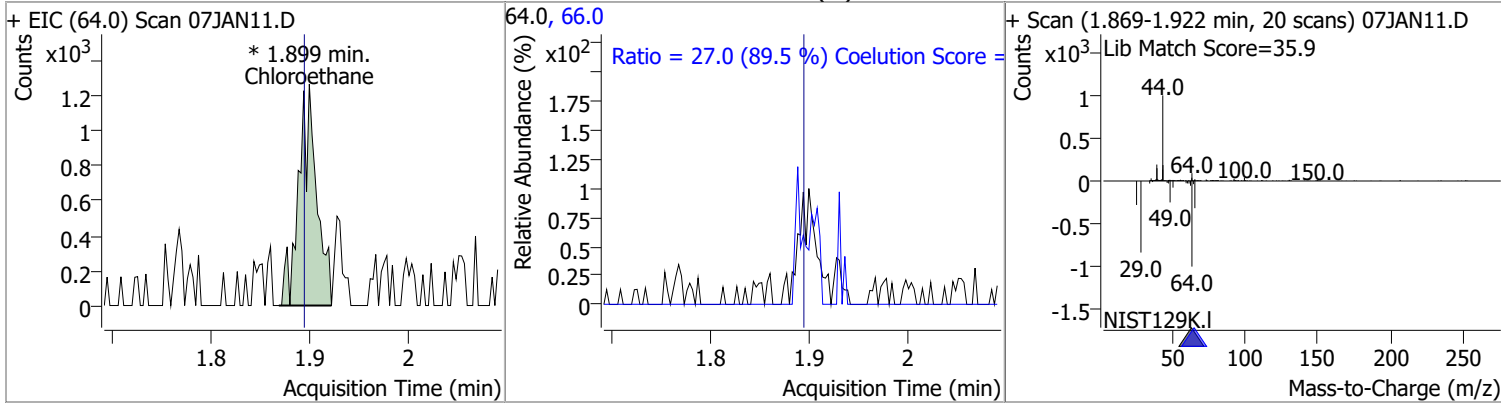


| Compound               | Conc. | Exp RT | QIon  | Exp Ratio |
|------------------------|-------|--------|-------|-----------|
| Trichlorofluoromethane | N.D.  | 2.14   | 103.0 | 64.2      |

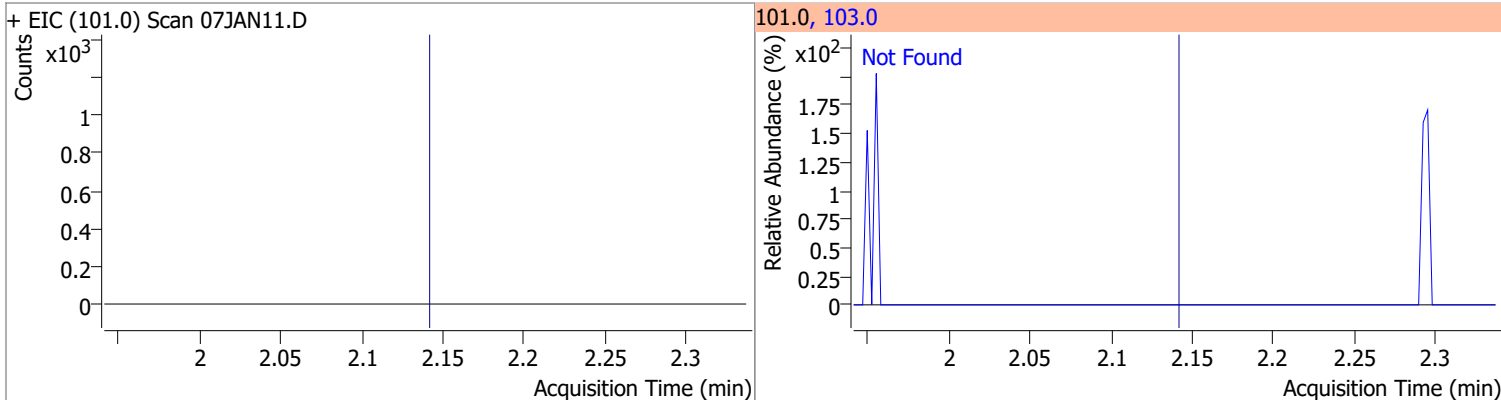



| Compound           | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethene | N.D.  | 2.70   | 61.0 | 180.3     | 63.0 | 56.7      |

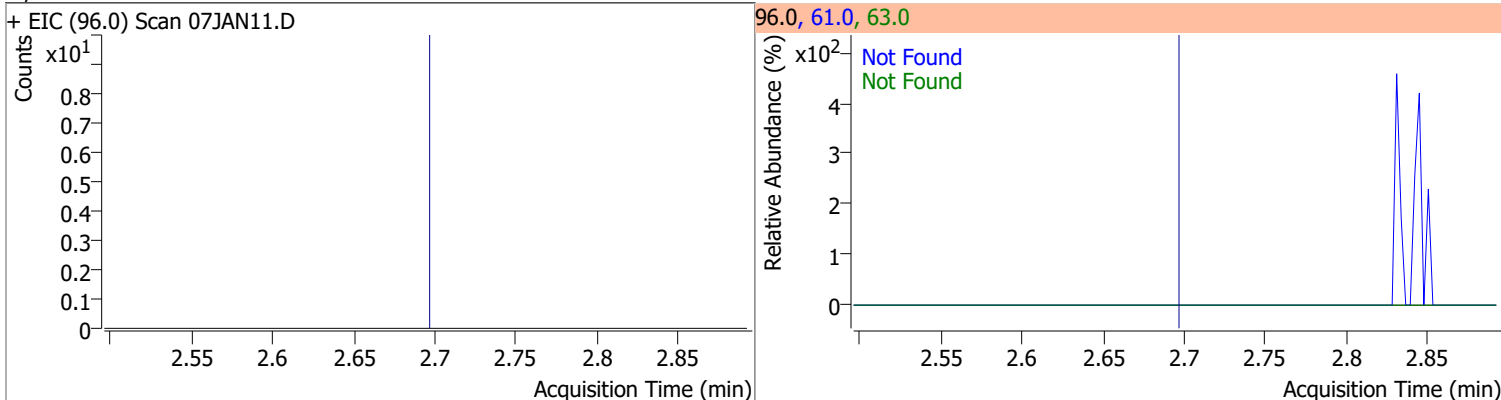



| Compound           | Conc.  | RT   | Dev(Min) | Resp.    | QIon | QRatio | Lower | Upper |
|--------------------|--------|------|----------|----------|------|--------|-------|-------|
| Methylene chloride | 1.0727 | 3.33 | 0.00     | 1285 (m) | 84.0 | 81.6   | 36.9  | 96.9  |
|                    |        |      |          |          | 86.0 | 54.6   | 14.3  | 74.3  |

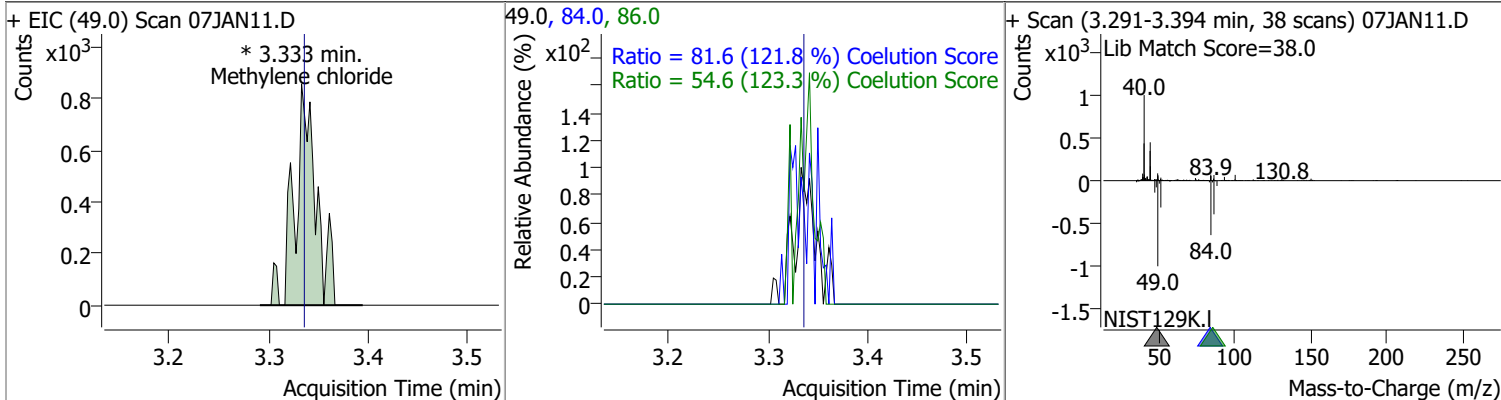

# Quantitation Results Report (QT Reviewed)

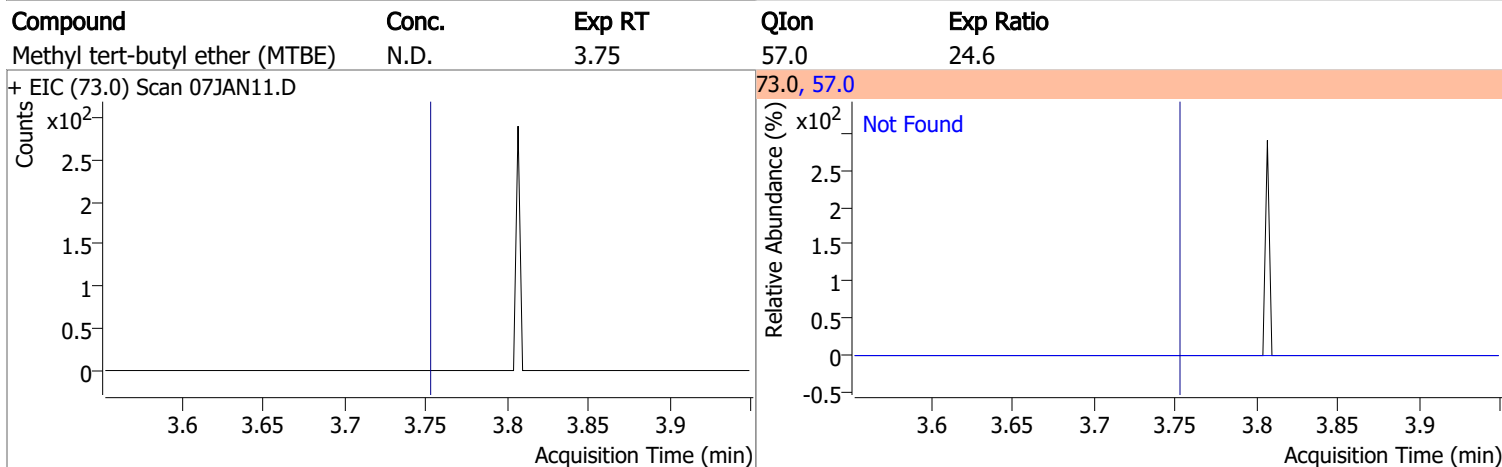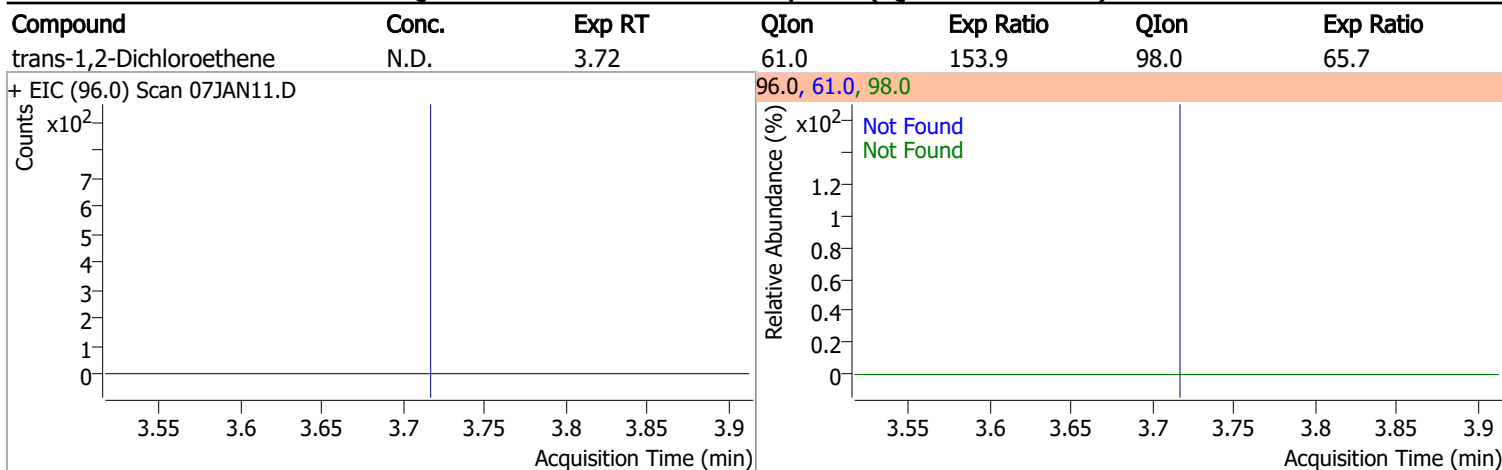


| Compound           | Conc.  | RT   | Dev(Min) | Resp.   | QIon | QRatio | Lower | Upper |
|--------------------|--------|------|----------|---------|------|--------|-------|-------|
| 1,1-Dichloroethane | 0.6175 | 4.38 | 0.00     | 953 (m) | 65.0 | 18.6   | 2.1   | 62.1  |
|                    |        |      |          |         | 83.0 | 3.7    | 0.0   | 43.7  |

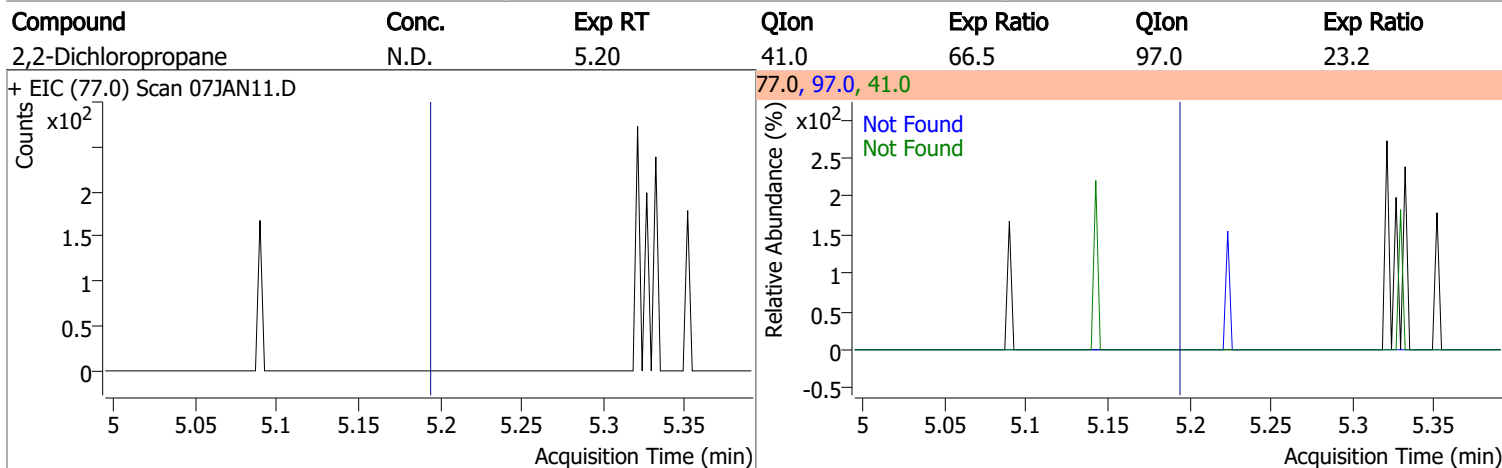




# Quantitation Results Report (QT Reviewed)


| Compound               | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|------------------------|-------|--------|------|-----------|------|-----------|
| cis-1,2-Dichloroethene | N.D.  | 5.22   | 61.0 | 167.2     | 98.0 | 67.3      |




| Compound            | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| Methyl ethyl ketone | N.D.  | 5.28   | 72.0 | 21.3      |







| Compound           | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|
| Bromochloromethane | N.D.  | 5.52   | 49.0 | 182.9     |



| Compound   | Conc.  | RT   | Dev(Min) | Resp.   | QIon | QRatio | Lower | Upper |
|------------|--------|------|----------|---------|------|--------|-------|-------|
| Chloroform | 0.5057 | 5.65 | 0.00     | 777 (m) | 85.0 | 47.4   | 36.0  | 96.0  |




# Quantitation Results Report (QT Reviewed)

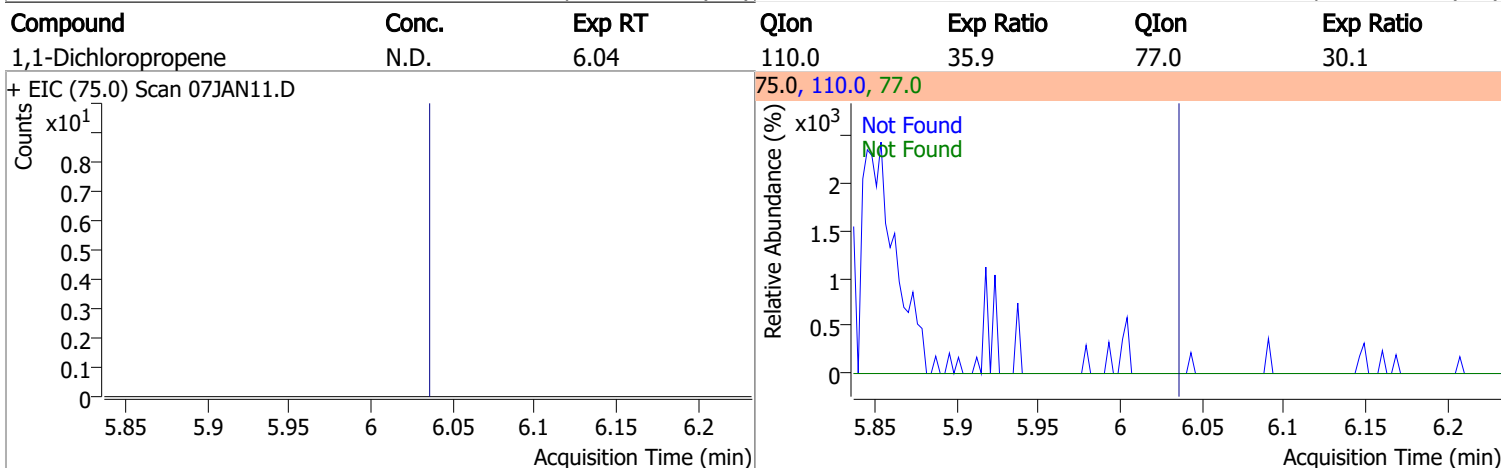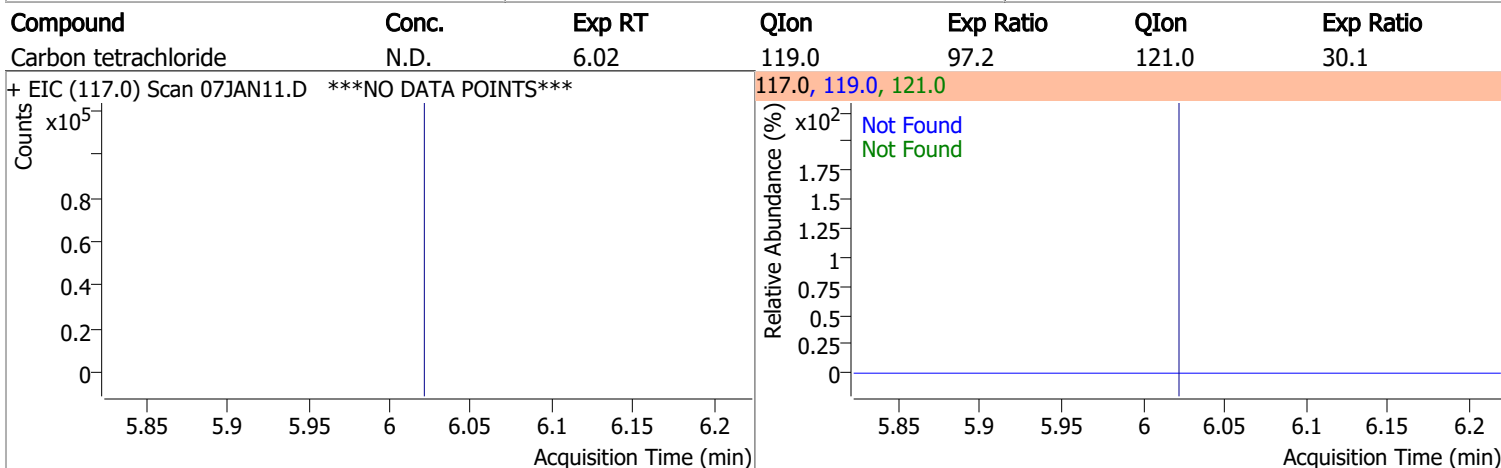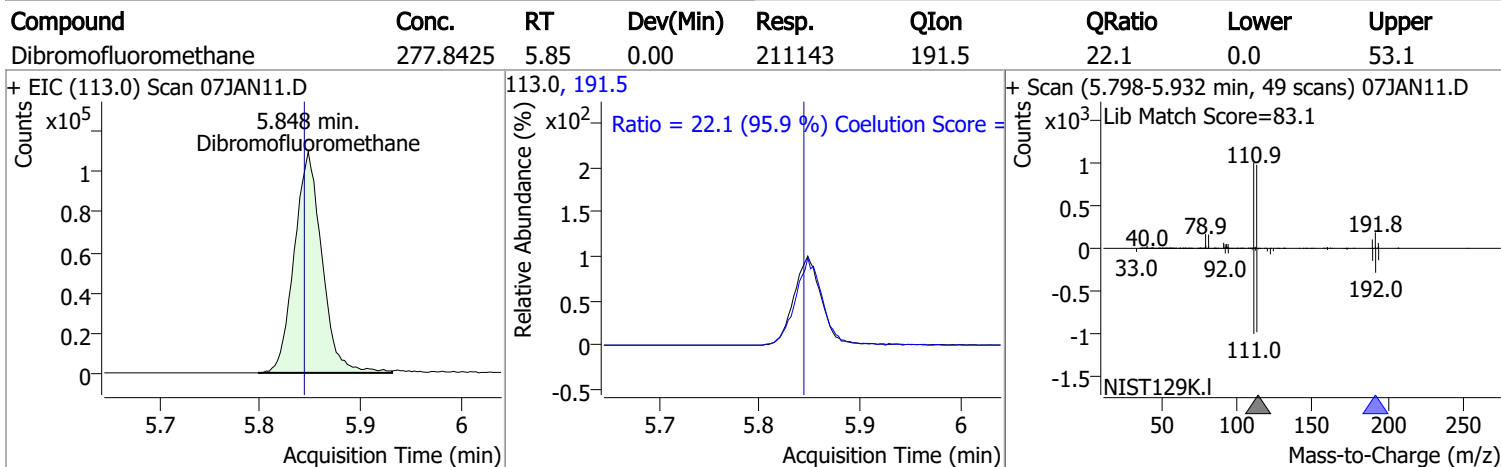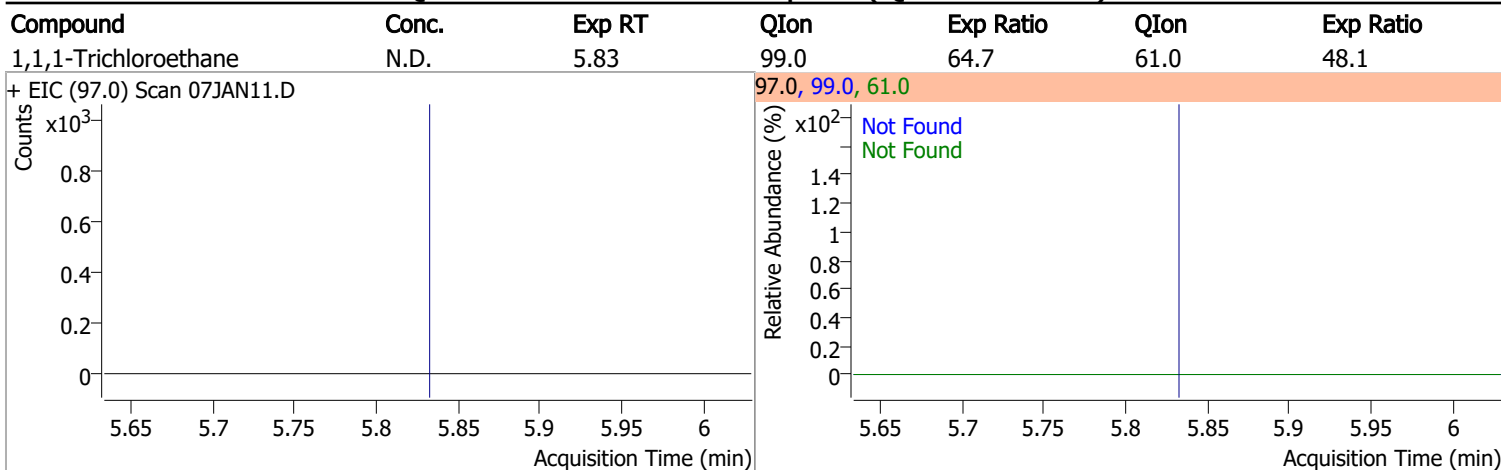


# Quantitation Results Report (QT Reviewed)


| Compound              | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 295.0174 | 6.23 | 0.00     | 96836 | 65.0 | 191.0  | 166.5 | 226.5 |

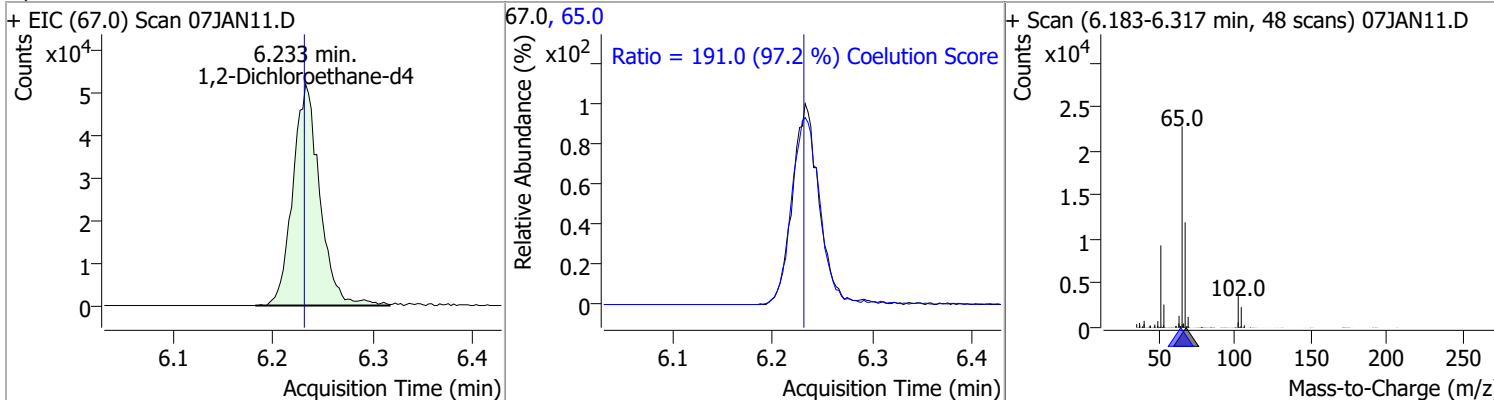


| Compound | Conc.  | RT   | Dev(Min) | Resp.    | QIon | QRatio | Lower | Upper |
|----------|--------|------|----------|----------|------|--------|-------|-------|
| Benzene  | 0.4371 | 6.28 | 0.00     | 1404 (m) | 77.0 | 11.1   | 0.0   | 53.5  |







| Compound           | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,2-Dichloroethane | N.D.  | 6.32   | 64.0 | 29.9      | 98.0 | 7.6       |

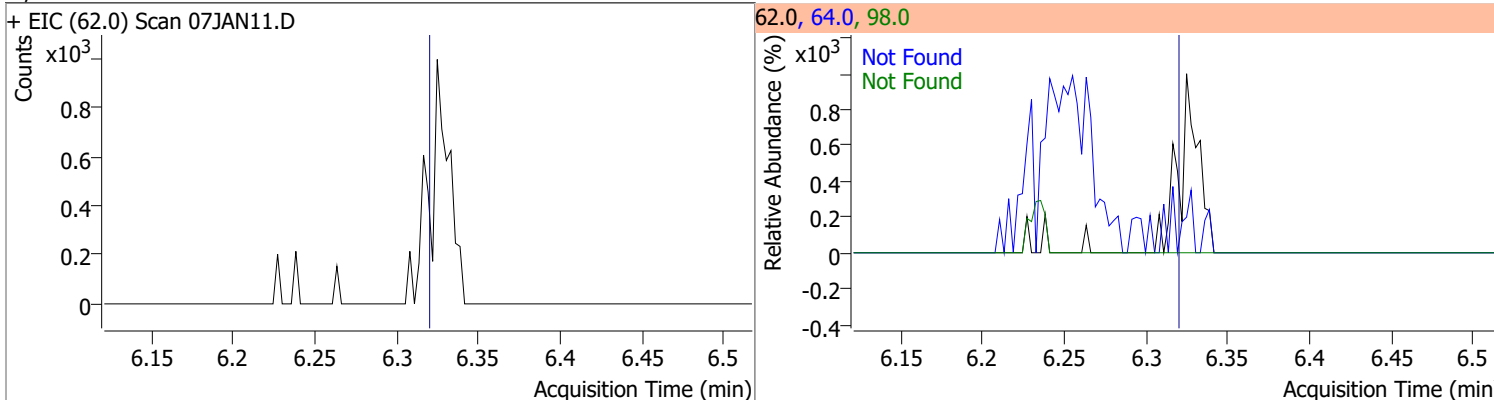

| Compound        | Conc. | Exp RT | QIon  | Exp Ratio | QIon | Exp Ratio |
|-----------------|-------|--------|-------|-----------|------|-----------|
| Trichloroethene | N.D.  | 7.03   | 130.0 | 101.5     | 97.0 | 64.1      |

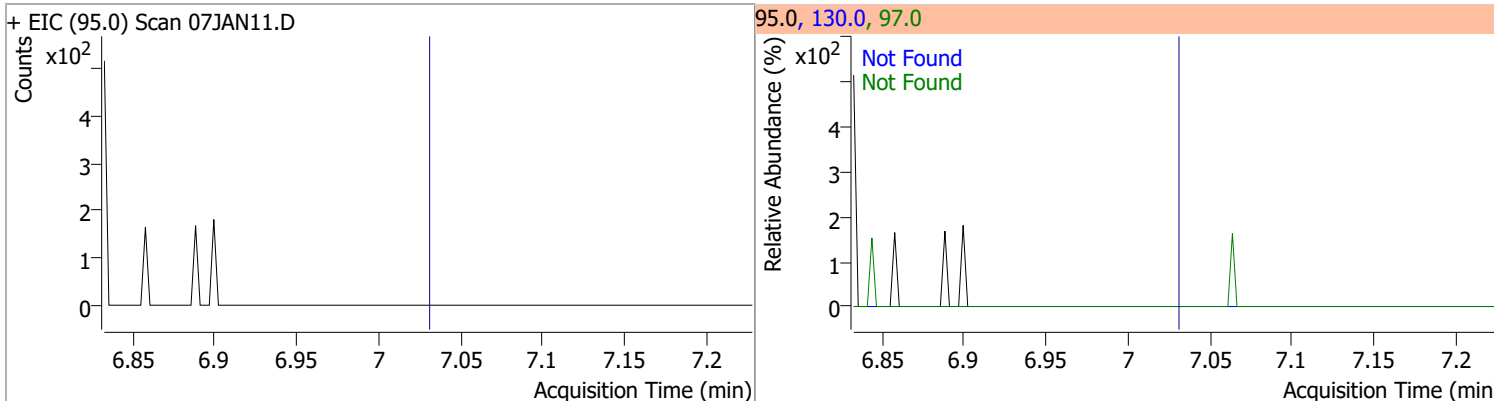


# Quantitation Results Report (QT Reviewed)

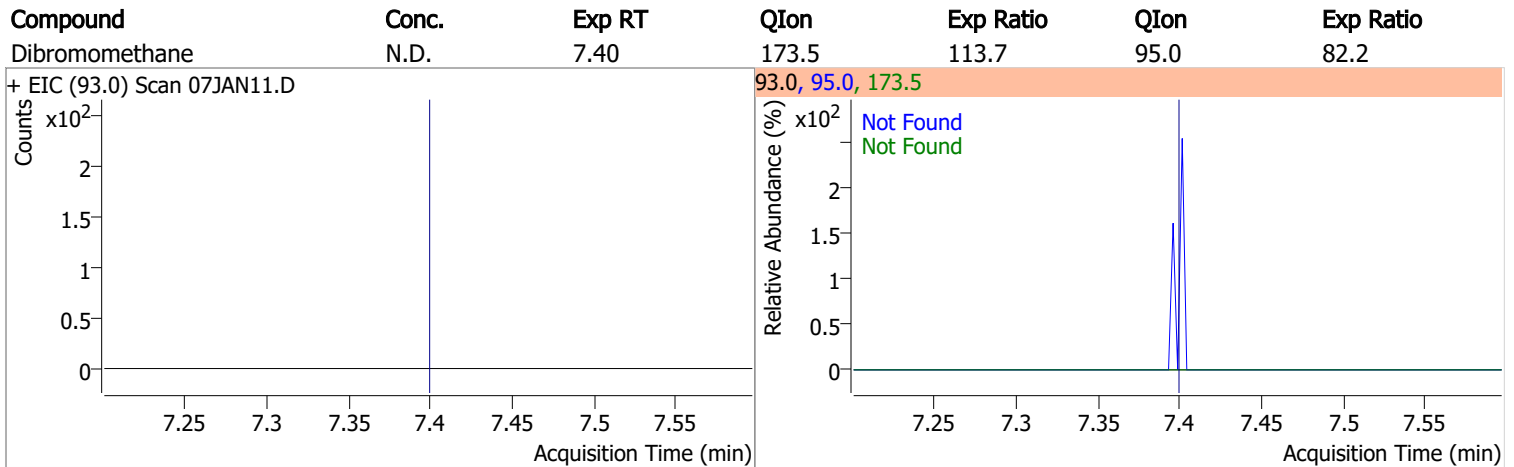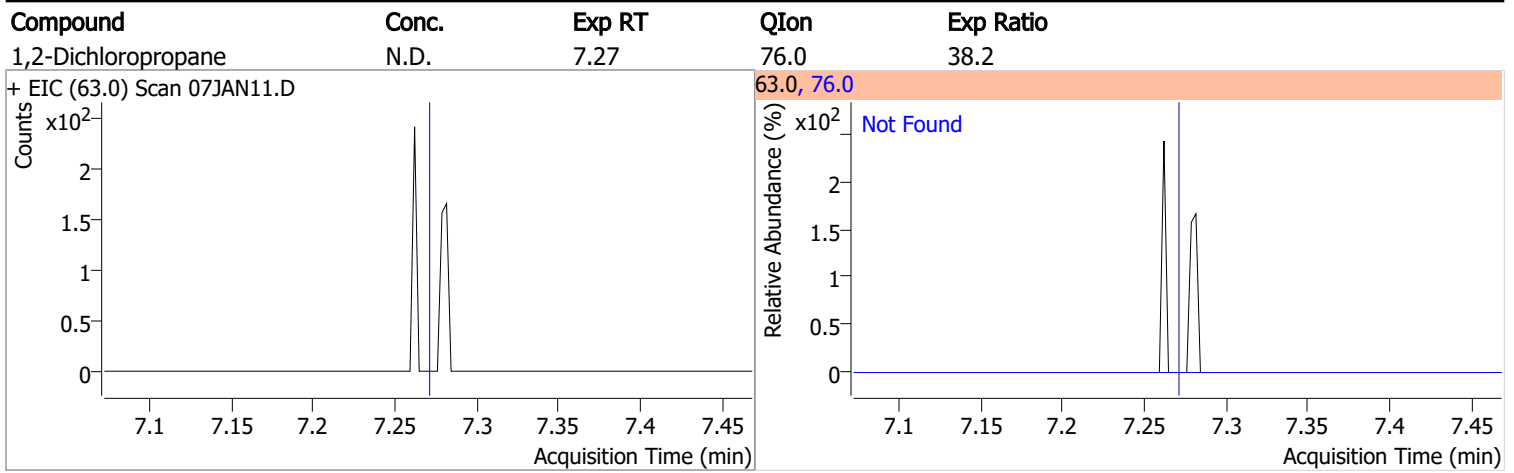


# Quantitation Results Report (QT Reviewed)


| Compound   | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 269.7270 | 8.32 | 0.00     | 811840 | 100.0 | 64.1   | 34.4  | 94.4  |
|            |          |      |          |        | 99.0  | 9.5    | 0.0   | 39.6  |

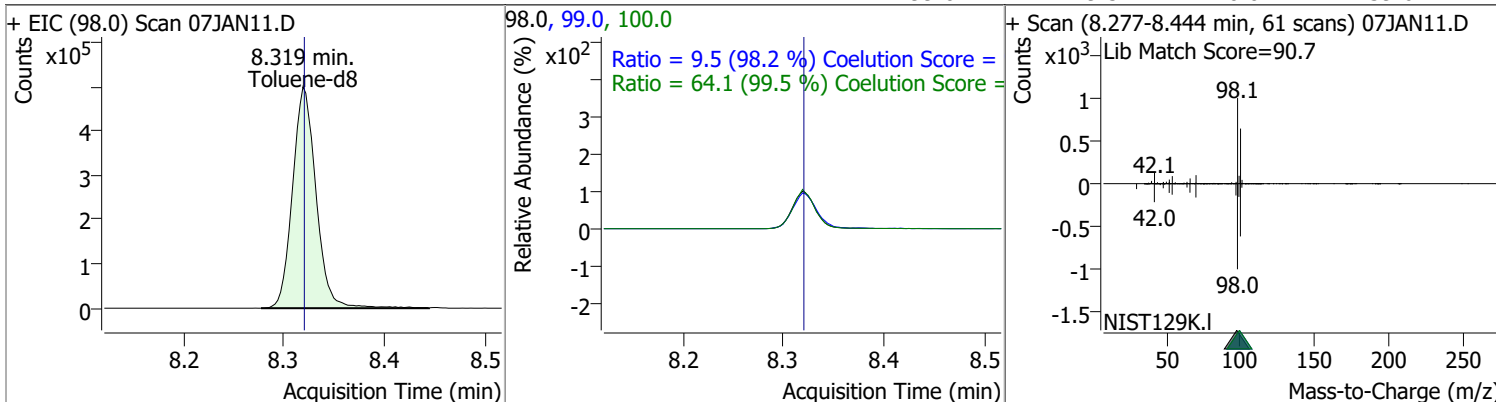


| Compound | Conc.  | RT   | Dev(Min) | Resp.   | QIon | QRatio | Lower | Upper |
|----------|--------|------|----------|---------|------|--------|-------|-------|
| Toluene  | 0.3436 | 8.40 | 0.01     | 699 (m) | 91.0 | 198.2  | 145.8 | 205.8 |

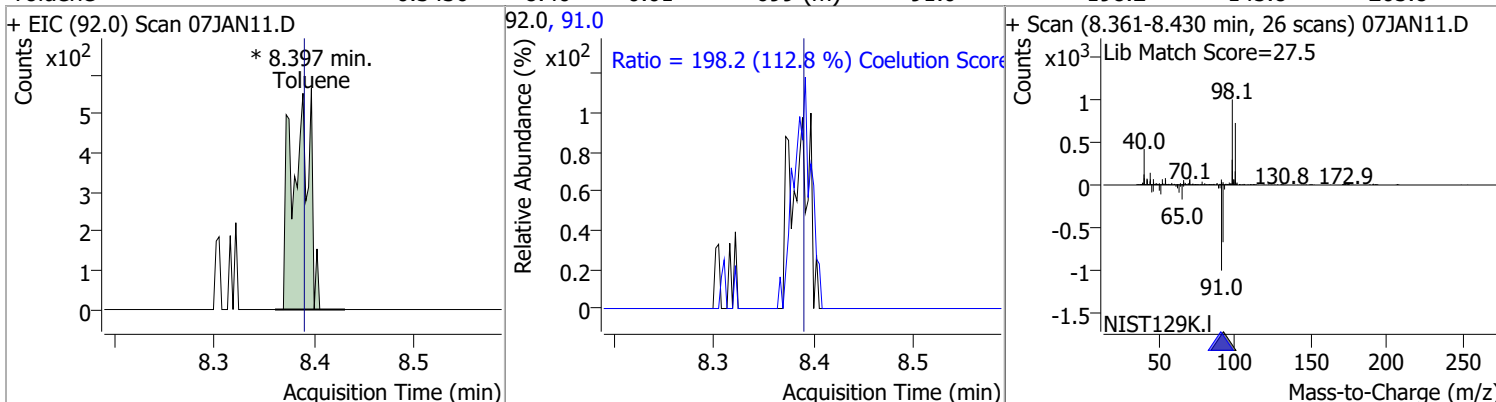

| Compound                  | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,3-Dichloropropene | N.D.  | 8.64   | 39.0 | 53.4      | 77.0 | 32.4      |

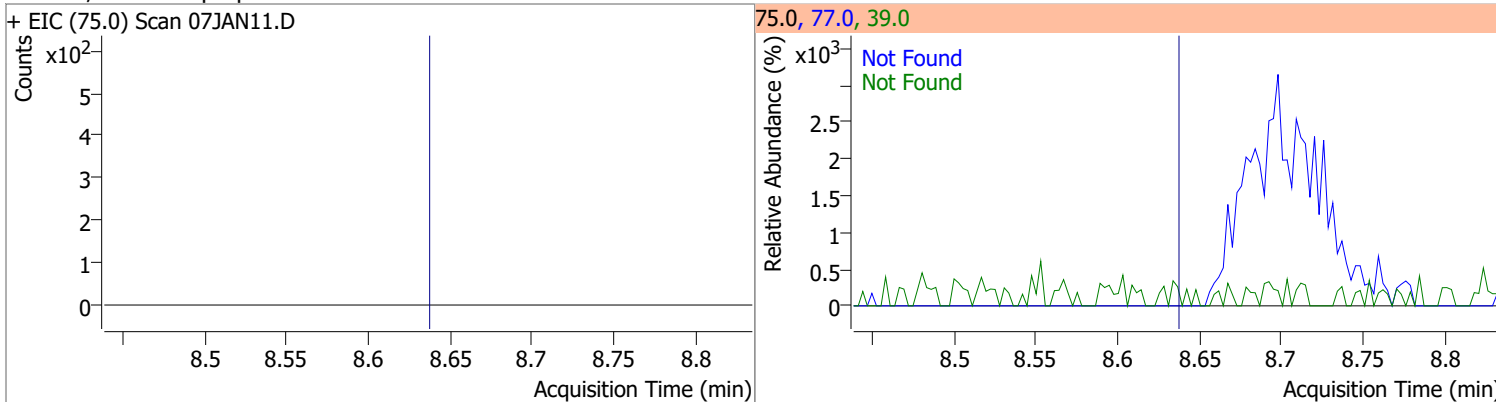


| Compound              | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|-------|----|----------|-------|------|--------|-------|-------|
| 1,1,2-Trichloroethane | 0     | 0  | 0        | 0     | 97.0 | 84.6   | 84.6  | 144.6 |
|                       |       |    |          |       | 85.0 | 37.6   | 37.6  | 97.6  |




# Quantitation Results Report (QT Reviewed)


| Compound          | Conc. | Exp RT | QIon  | Exp Ratio | QIon  | Exp Ratio |
|-------------------|-------|--------|-------|-----------|-------|-----------|
| Tetrachloroethene | N.D.  | 8.94   | 165.8 | 128.6     | 129.0 | 91.5      |




| Compound            | Conc.  | RT   | Dev(Min) | Resp.   | QIon | QRatio | Lower | Upper |
|---------------------|--------|------|----------|---------|------|--------|-------|-------|
| 1,3-Dichloropropane | 0.4005 | 8.98 | 0.00     | 319 (m) | 78.0 | 22.4   | 2.9   | 62.9  |







| Compound             | Conc. | Exp RT | QIon  | Exp Ratio |
|----------------------|-------|--------|-------|-----------|
| Chlorodibromomethane | N.D.  | 9.21   | 127.0 | 78.0      |



| Compound          | Conc. | Exp RT | QIon  | Exp Ratio |
|-------------------|-------|--------|-------|-----------|
| 1,2-Dibromoethane | N.D.  | 9.31   | 109.0 | 94.5      |




# Quantitation Results Report (QT Reviewed)

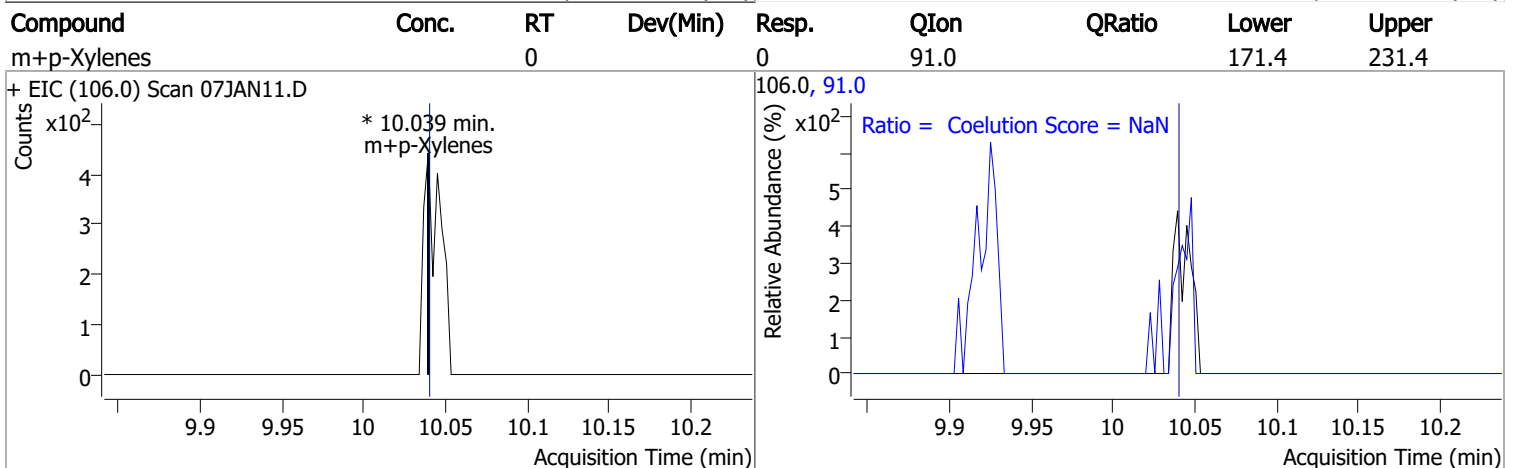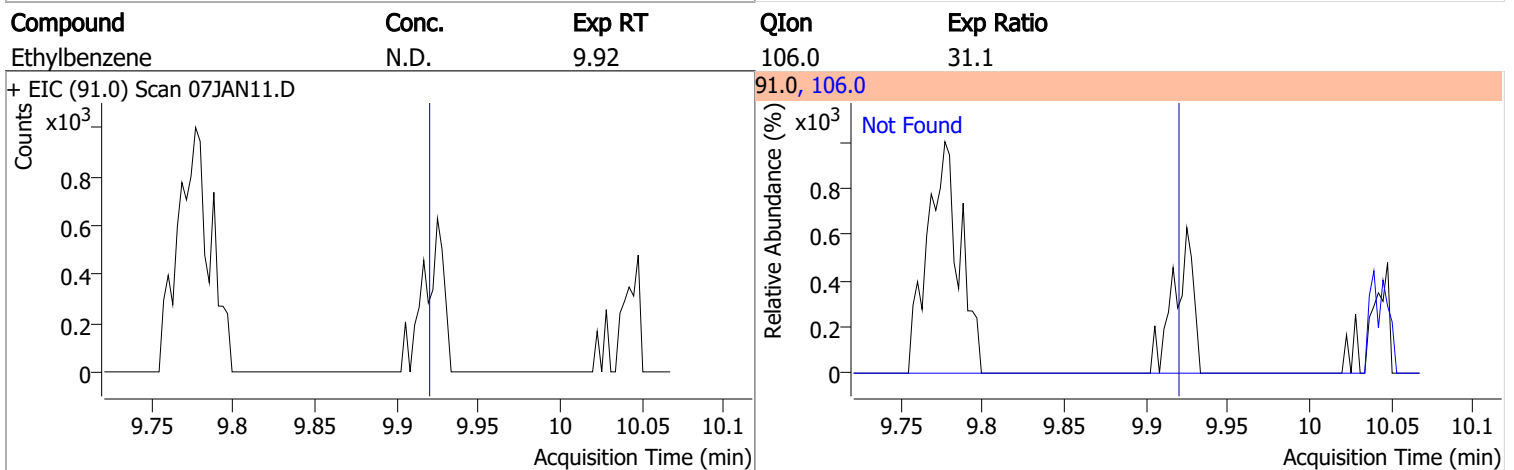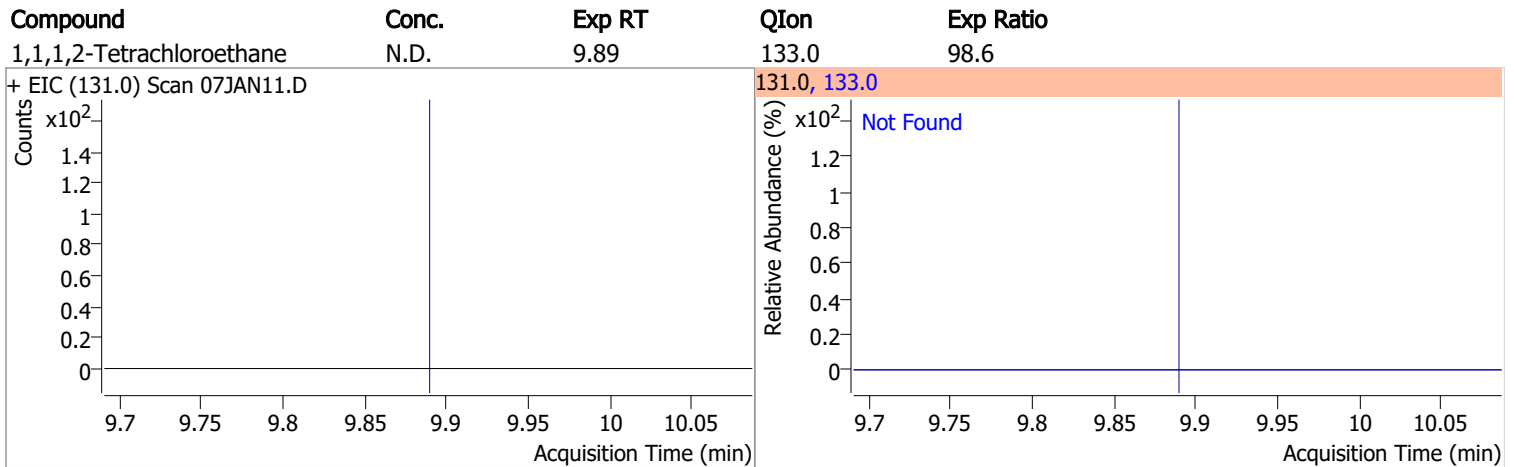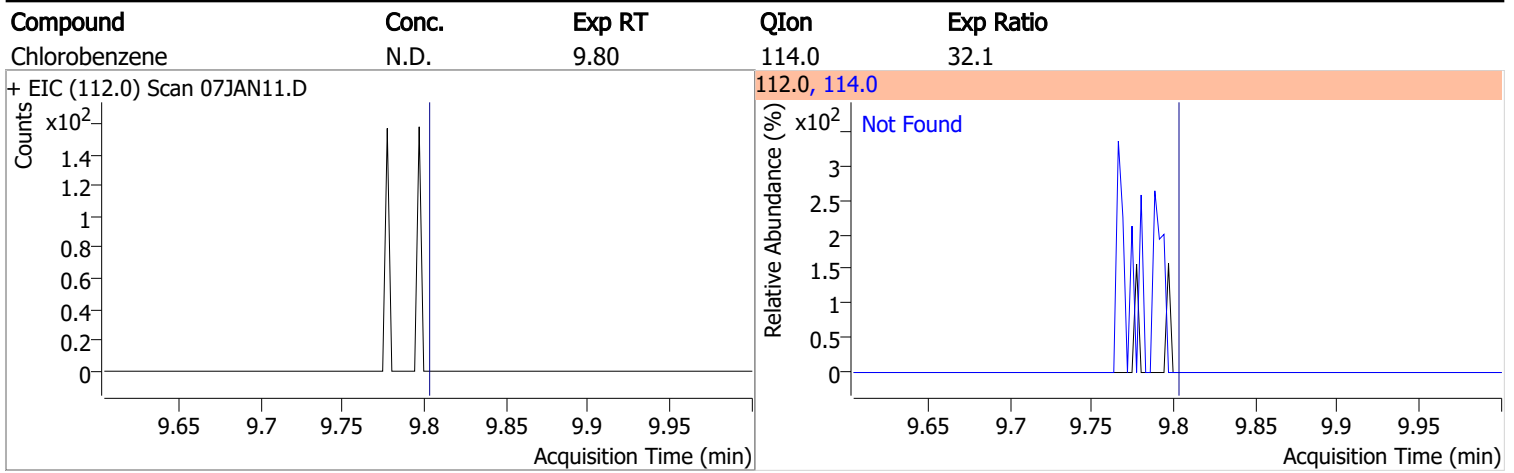


# Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|-------|----|----------|-------|------|--------|-------|-------|
| o-Xylene |       | 0  |          | 0     | 91.0 |        | 183.1 | 243.1 |

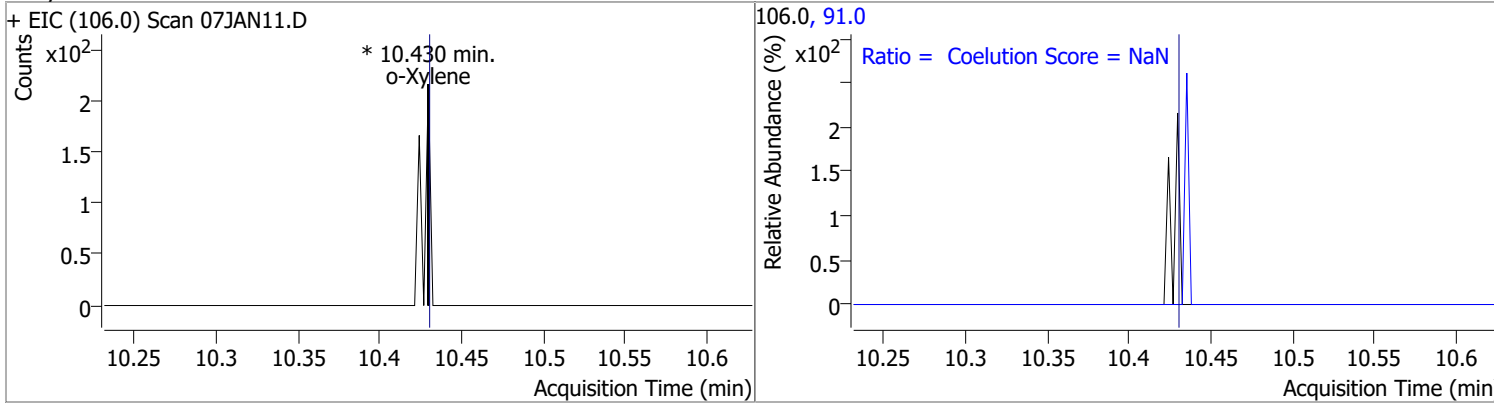


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------|-------|--------|------|-----------|
| Styrene  | N.D.  | 10.45  | 78.0 | 49.6      |

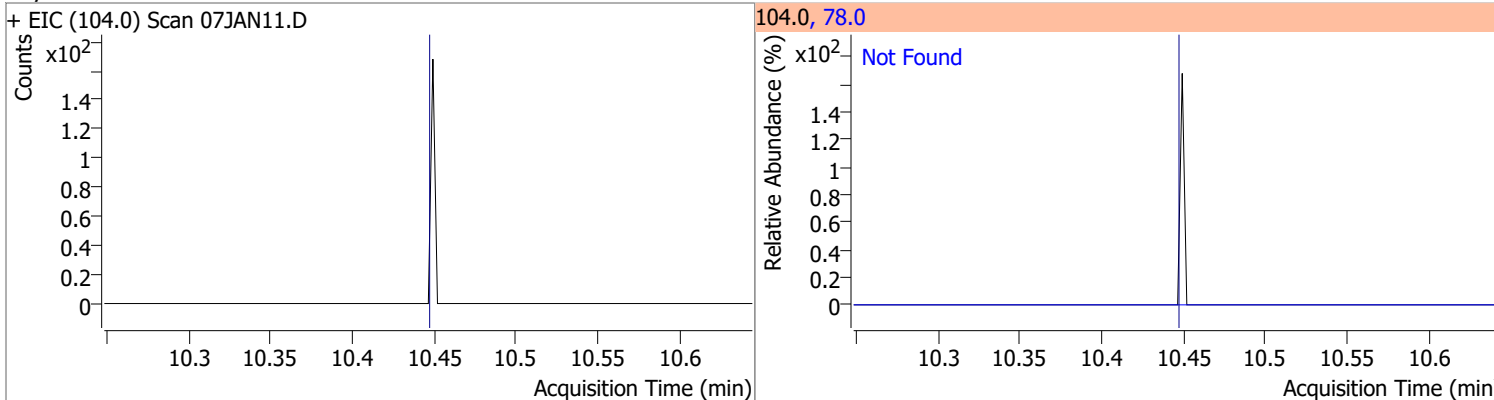

| Compound  | Conc. | Exp RT | QIon  | Exp Ratio | QIon  | Exp Ratio |
|-----------|-------|--------|-------|-----------|-------|-----------|
| Bromoform | N.D.  | 10.63  | 170.5 | 52.1      | 174.5 | 50.1      |

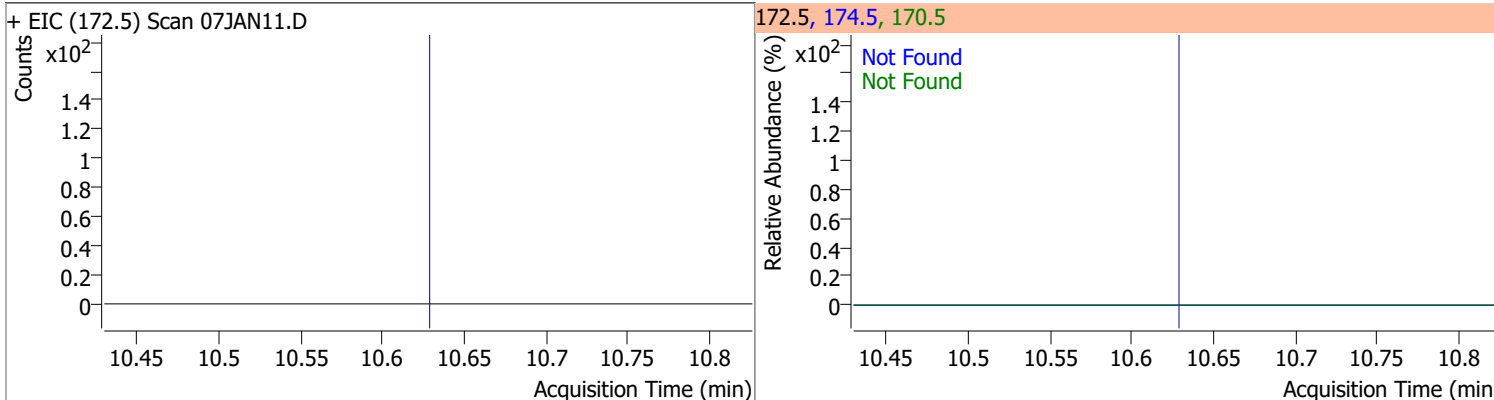


| Compound             | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 270.6993 | 10.95 | 0.00     | 237586 | 174.0 | 94.5   | 61.7  | 121.7 |
|                      |          |       |          |        | 176.0 | 92.2   | 60.6  | 120.6 |

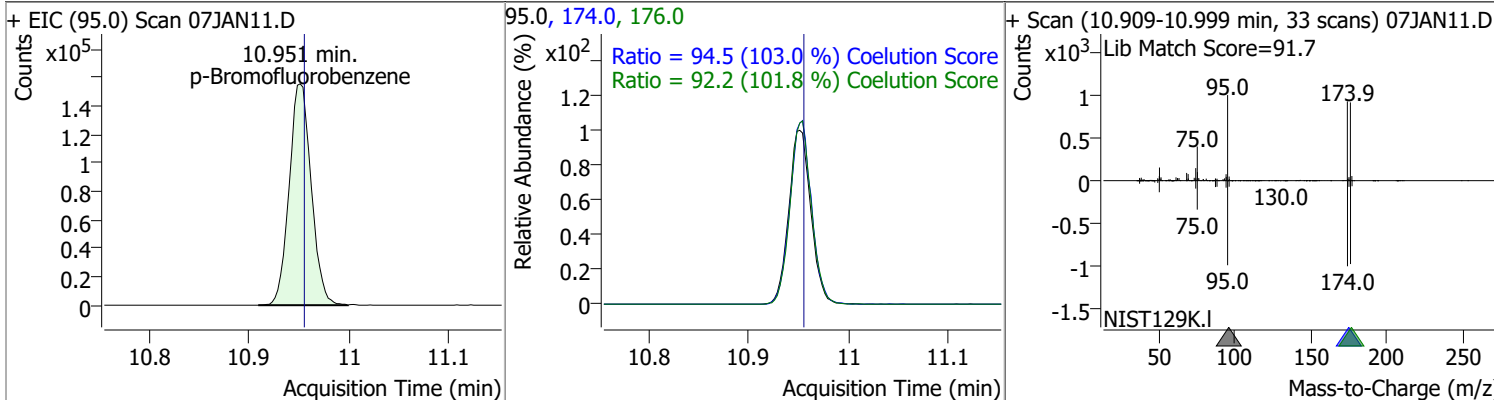




# Quantitation Results Report (QT Reviewed)


| Compound     | Conc. | Exp RT | QIon | Exp Ratio | QIon  | Exp Ratio |
|--------------|-------|--------|------|-----------|-------|-----------|
| Bromobenzene | N.D.  | 11.09  | 77.0 | 145.7     | 158.0 | 96.5      |




| Compound                  | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------------|-------|--------|------|-----------|
| 1,1,2,2-Tetrachloroethane | N.D.  | 11.12  | 85.0 | 66.2      |











| Compound               | Conc. | Exp RT | QIon  | Exp Ratio |
|------------------------|-------|--------|-------|-----------|
| 1,2,3-Trichloropropane | N.D.  | 11.15  | 112.0 | 63.5      |



| Compound        | Conc. | Exp RT | QIon | Exp Ratio |
|-----------------|-------|--------|------|-----------|
| 2-Chlorotoluene | N.D.  | 11.29  | 91.0 | 282.3     |




# Quantitation Results Report (QT Reviewed)
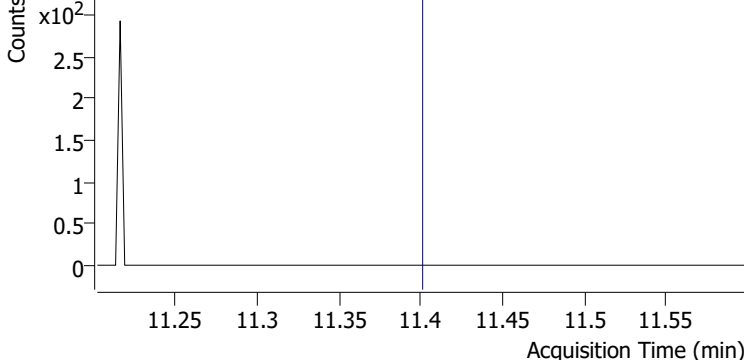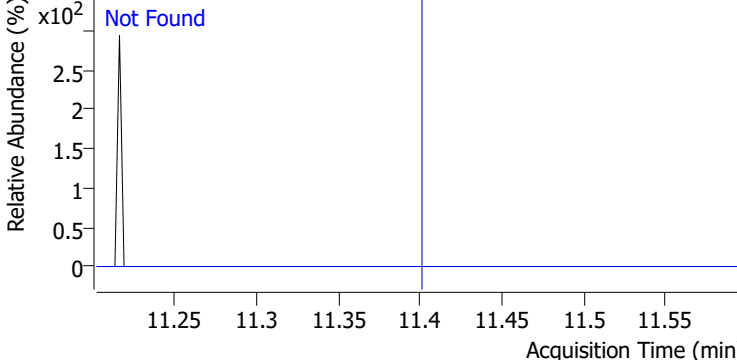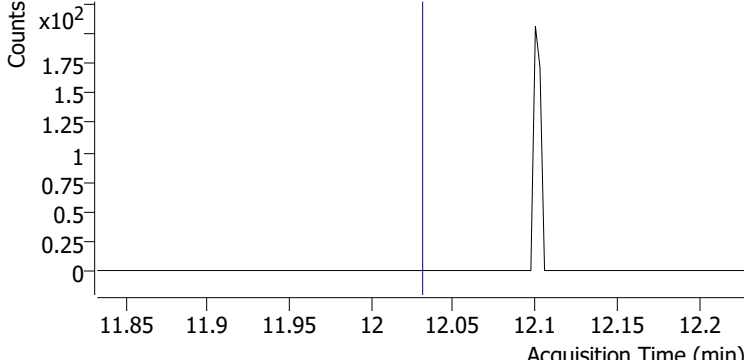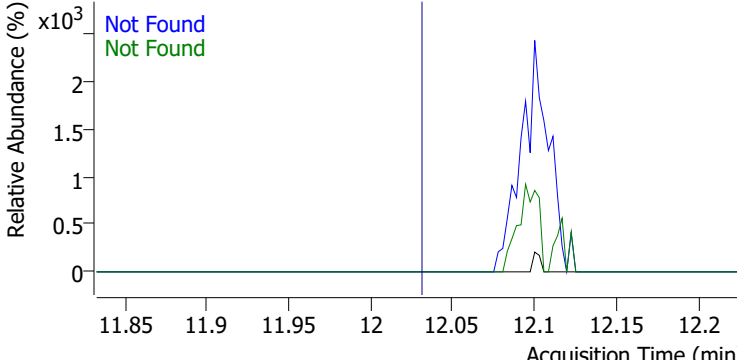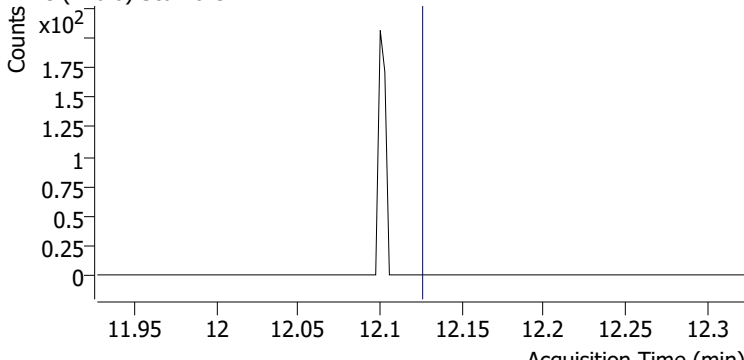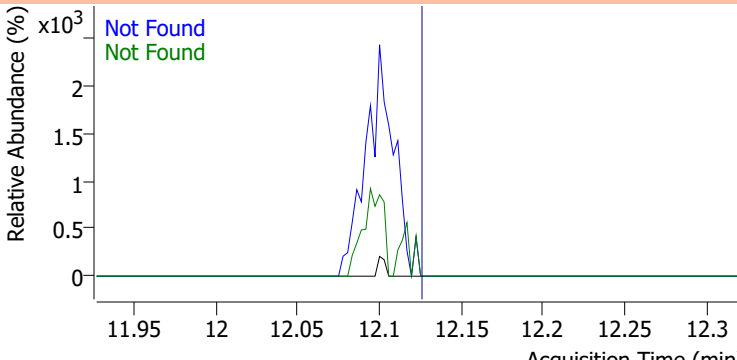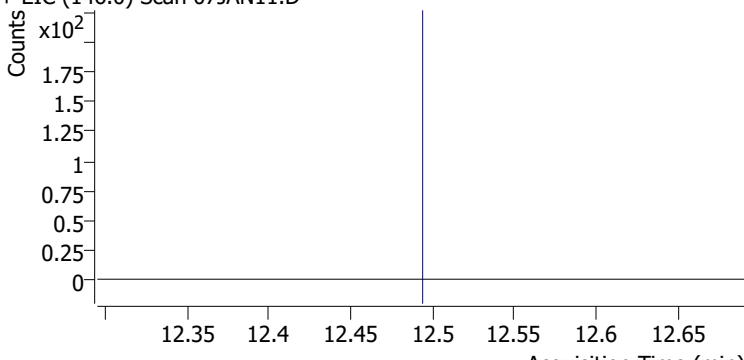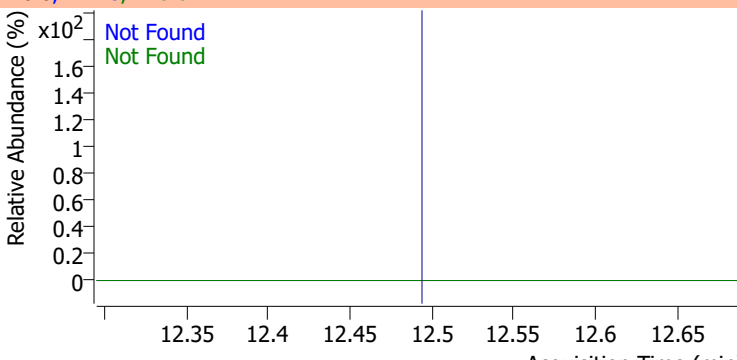
| Compound                                                                           | Conc. | Exp RT | QIon                                                                                 | Exp Ratio |      |           |
|------------------------------------------------------------------------------------|-------|--------|--------------------------------------------------------------------------------------|-----------|------|-----------|
| 4-Chlorotoluene                                                                    | N.D.  | 11.40  | 126.0                                                                                | 31.7      |      |           |
| + EIC (91.0) Scan 07JAN11.D                                                        |       |        | 91.0, 126.0                                                                          |           |      |           |
|    |       |        |    |           |      |           |
| 1,3-Dichlorobenzene                                                                | N.D.  | 12.03  | 148.0                                                                                | 63.6      | QIon | Exp Ratio |
| + EIC (146.0) Scan 07JAN11.D                                                       |       |        | 146.0, 111.0, 148.0                                                                  |           |      |           |
|   |       |        |   |           |      |           |
| 1,4-Dichlorobenzene                                                                | N.D.  | 12.13  | 148.0                                                                                | 63.1      | QIon | Exp Ratio |
| + EIC (146.0) Scan 07JAN11.D                                                       |       |        | 146.0, 111.0, 148.0                                                                  |           |      |           |
|  |       |        |  |           |      |           |
| 1,2-Dichlorobenzene                                                                | N.D.  | 12.49  | 148.0                                                                                | 63.9      | QIon | Exp Ratio |
| + EIC (146.0) Scan 07JAN11.D                                                       |       |        | 146.0, 111.0, 148.0                                                                  |           |      |           |
|  |       |        |  |           |      |           |

# Quantitation Results Report (QT Reviewed)

|                |                                     |                   |                       |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File      | 07JAN12.D                           | Operator          | MSC                   |
| Acq. Method    | 5975CACQF.M                         | Acq. Date-Time    | 1/7/2022 2:41:20 PM   |
| Sample Name    | B22010213-002C                      | Instrument        | VOA5975C              |
| Vial           | 12                                  | Multiplier        | 1.00                  |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m  | Comment           |                       |
| Tune File      | BFB_Atune3.u                        | Tune Date         | 10/11/2021 4:02:00 PM |
| Batch Name     | VG010722_8260B.batch.bin            | Last Calib Update | 3/2/2022 10:41:44 AM  |
| Ref Library    | \\MASSHUNTER\Org\Library\NIST129K.l |                   |                       |

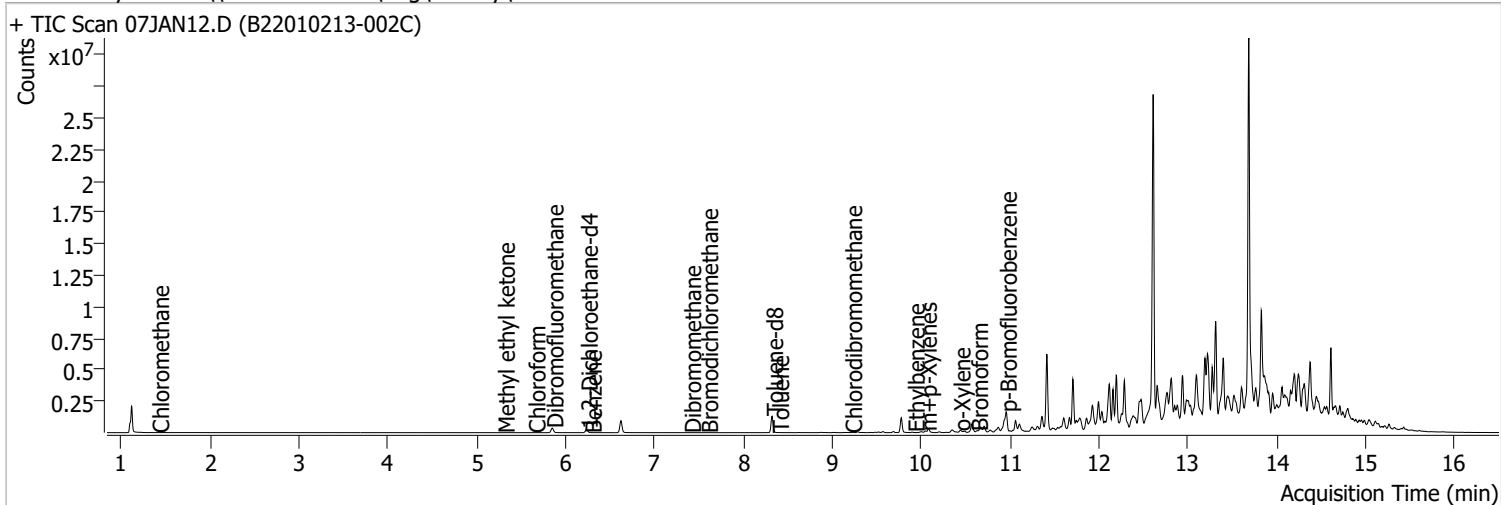





| Compound                           | RT                   | QIon  | Resp.  | Conc.              | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|--------------------|-------|----------|
| <b>Internal Standards</b>          |                      |       |        |                    |       |          |
| M Fluorobenzene                    | 6.620                | 96.0  | 797906 | 250.0000           | ng    | -0.003   |
| M Chlorobenzene-d5                 | 9.774                | 82.0  | 317458 | 250.0000           | ng    | 0.003    |
| M 1,4-Dichlorobenzene-d4           | 12.100               | 152.0 | 260553 | 250.0000           | ng    | 0.000    |
| <b>System Monitoring Compounds</b> |                      |       |        |                    |       |          |
| S Dibromofluoromethane             | 5.851                | 113.0 | 209602 | 278.8342           | ng    | 0.005    |
| Spiked Amount: 250.000             | Range: 80.0 - 119.0% |       |        | Recovery = 111.53% |       |          |
| S 1,2-Dichloroethane-d4            | 6.236                | 67.0  | 94741  | 291.7947           | ng    | 0.003    |
| Spiked Amount: 250.000             | Range: 81.0 - 118.0% |       |        | Recovery = 116.72% |       |          |
| S Toluene-d8                       | 8.321                | 98.0  | 800313 | 261.6097           | ng    | 0.003    |
| Spiked Amount: 250.000             | Range: 89.0 - 112.0% |       |        | Recovery = 104.64% |       |          |
| S p-Bromofluorobenzene             | 10.951               | 95.0  | 258089 | 270.3807           | ng    | -0.003   |
| Spiked Amount: 250.000             | Range: 85.0 - 114.0% |       |        | Recovery = 108.15% |       |          |
| <b>Target Compounds</b>            |                      |       |        |                    |       |          |
| T Dichlorodifluoromethane          | 0.000                |       | 0      | N.D.               |       |          |
| T Chloromethane                    | 1.417                | 50.0  | 854    | 0.6730             | ng    | m 63     |
| T Vinyl chloride                   | 0.000                |       | 0      | N.D.               |       |          |
| T Bromomethane                     | 0.000                |       | 0      | N.D.               |       |          |
| T Chloroethane                     | 0.000                |       | 0      | N.D.               |       |          |
| T Trichlorofluoromethane           | 0.000                |       | 0      | N.D.               |       |          |
| T 1,1-Dichloroethene               | 0.000                |       | 0      | N.D.               |       |          |
| T Methylene chloride               | 0.000                |       | 0      | N.D.               |       |          |
| T trans-1,2-Dichloroethene         | 0.000                |       | 0      | N.D.               |       |          |
| T Methyl tert-butyl ether (MTBE)   | 0.000                |       | 0      | N.D.               |       |          |
| T 1,1-Dichloroethane               | 0.000                |       | 0      | N.D.               |       |          |
| T 2,2-Dichloropropane              | 0.000                |       | 0      | N.D.               |       |          |
| T cis-1,2-Dichloroethene           | 0.000                |       | 0      | N.D.               |       |          |
| T Methyl ethyl ketone              | 5.304                | 43.0  | 565    | 5.0179             | ng    | m 97     |
| T Bromochloromethane               | 0.000                |       | 0      | N.D.               |       |          |
| T Chloroform                       | 5.647                | 83.0  | 1655   | 1.0896             | ng    | m 89     |

# Quantitation Results Report (QT Reviewed)

| Compound                    | RT     | QIon  | Resp. | Conc.  | Units |    | Dev(Min) |
|-----------------------------|--------|-------|-------|--------|-------|----|----------|
| T 1,1,1-Trichloroethane     | 0.000  |       | 0     | N.D.   |       |    |          |
| T Carbon tetrachloride      | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,1-Dichloropropene       | 0.000  |       | 0     | N.D.   |       |    |          |
| T Benzene                   | 6.280  | 78.0  | 409   | 0.1289 | ng    | m  | 74       |
| T 1,2-Dichloroethane        | 0.000  |       | 0     | N.D.   |       |    |          |
| T Trichloroethene           | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,2-Dichloropropane       | 0.000  |       | 0     | N.D.   |       |    |          |
| T Dibromomethane            | 7.398  | 93.0  | 111   | 0.3122 | ng    | m  | 86       |
| T Bromodichloromethane      | 7.591  | 83.0  | 654   | 0.6660 | ng    | m  | 93       |
| T cis-1,3-Dichloropropene   | 0.000  |       | 0     | N.D.   |       |    |          |
| T Toluene                   | 8.388  | 92.0  | 493   | 0.2388 | ng    | m  | 97       |
| T trans-1,3-Dichloropropene | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,1,2-Trichloroethane     | 0.000  |       | 0     | N.D.   |       |    |          |
| T Tetrachloroethene         | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,3-Dichloropropane       | 0.000  |       | 0     | N.D.   |       |    |          |
| T Chlorodibromomethane      | 9.211  | 129.0 | 1602  | 2.4889 | ng    | m  | 80       |
| T 1,2-Dibromoethane         | 0.000  |       | 0     | N.D.   |       |    |          |
| T Chlorobenzene             | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,1,1,2-Tetrachloroethane | 0.000  |       | 0     | N.D.   |       |    |          |
| T Ethylbenzene              | 9.917  | 91.0  | 1441  | 0.3673 | ng    | m  | 62       |
| T m+p-Xylenes               | 10.050 | 106.0 | 1346  | 0.8826 | ng    | m  | 82       |
| T o-Xylene                  | 10.430 | 106.0 | 3810  | 2.8067 | ng    |    | 82       |
| T Styrene                   | 0.000  |       | 0     | N.D.   |       |    |          |
| T Bromoform                 | 10.628 | 172.5 | 2322  | 6.9642 | ng    |    | 98       |
| T Bromobenzene              | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,1,2,2-Tetrachloroethane | 11.099 | 83.0  | 0     |        | ng    | md | 1        |
| T 1,2,3-Trichloropropane    | 11.146 | 110.0 | 0     |        | ng    | md | 1        |
| T 2-Chlorotoluene           | 0.000  |       | 0     | N.D.   |       |    |          |
| T 4-Chlorotoluene           | 11.392 | 91.0  | 0     |        | ng    | md | 1        |
| T 1,3-Dichlorobenzene       | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,4-Dichlorobenzene       | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,2-Dichlorobenzene       | 0.000  |       | 0     | N.D.   |       |    |          |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (\*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

# Quantitation Results Report (QT Reviewed)

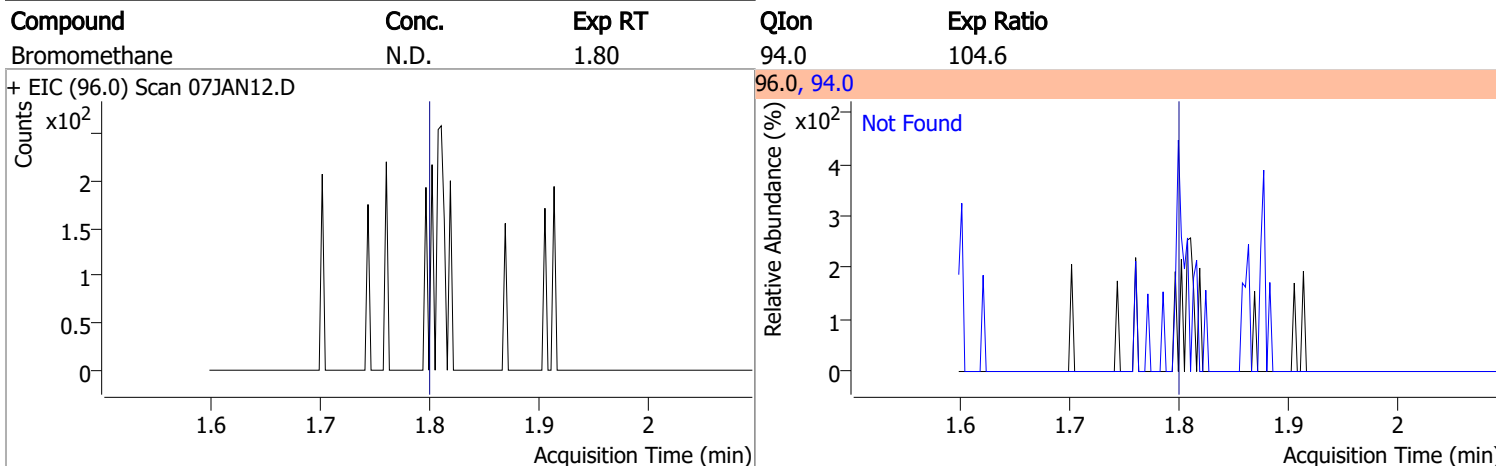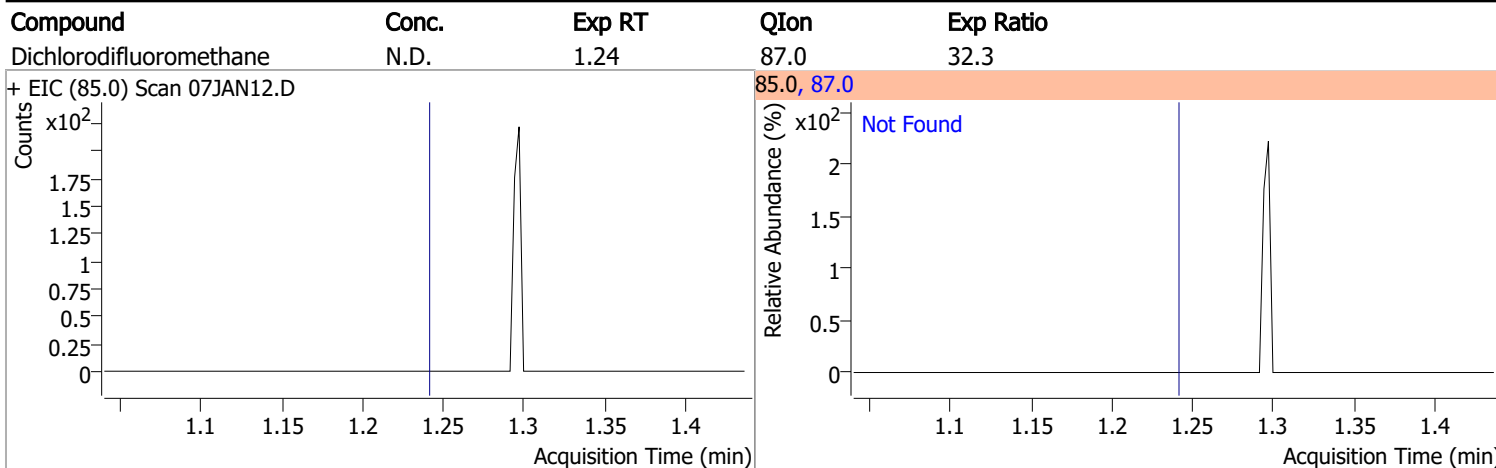


# Quantitation Results Report (QT Reviewed)


| Compound     | Conc. | Exp RT | QIon | Exp Ratio |
|--------------|-------|--------|------|-----------|
| Chloroethane | N.D.  | 1.89   | 66.0 | 30.1      |

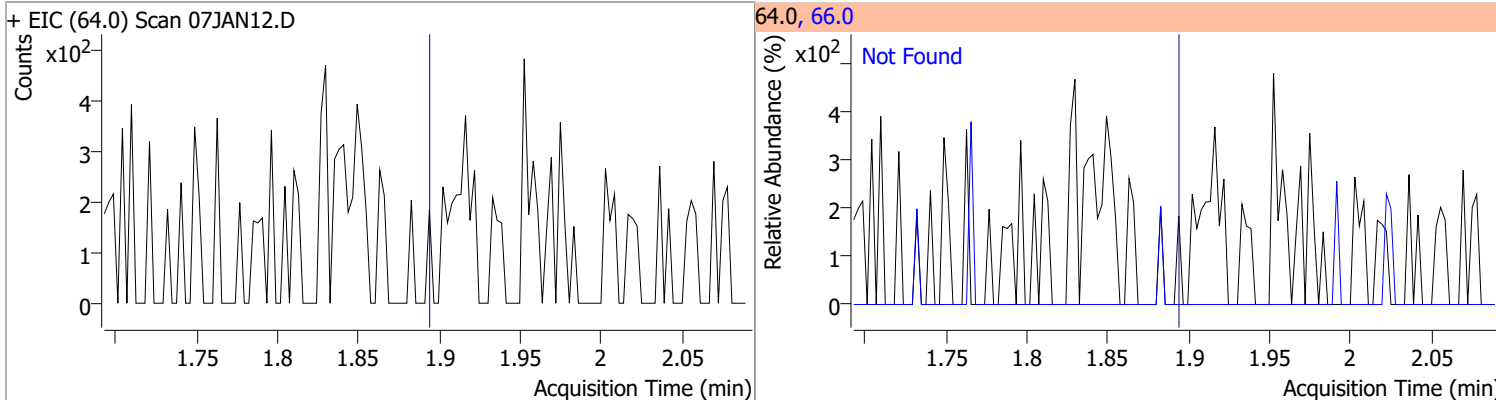


| Compound               | Conc. | Exp RT | QIon  | Exp Ratio |
|------------------------|-------|--------|-------|-----------|
| Trichlorofluoromethane | N.D.  | 2.14   | 103.0 | 64.2      |

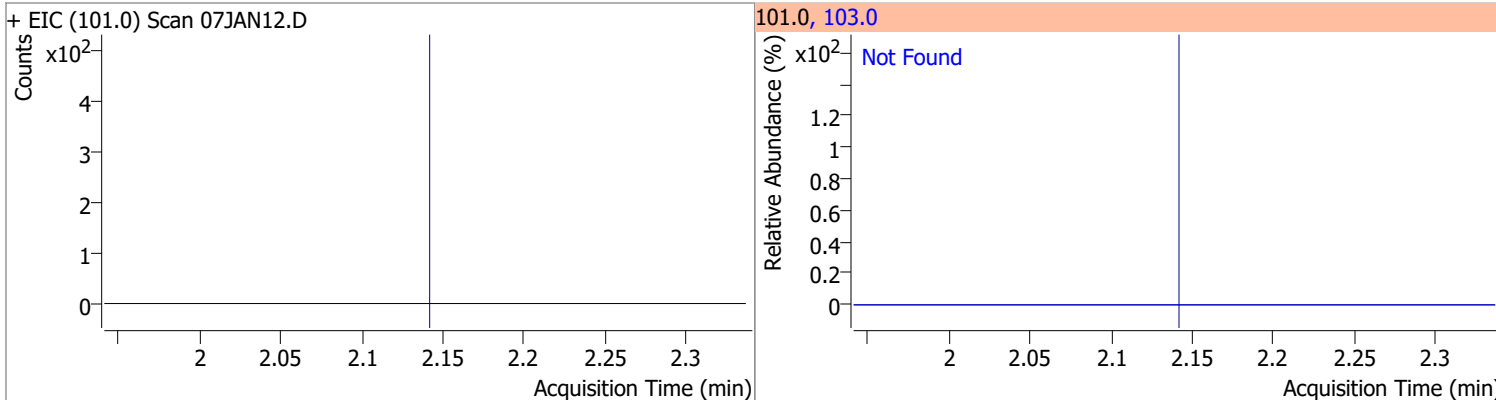









| Compound           | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethene | N.D.  | 2.70   | 61.0 | 180.3     | 63.0 | 56.7      |

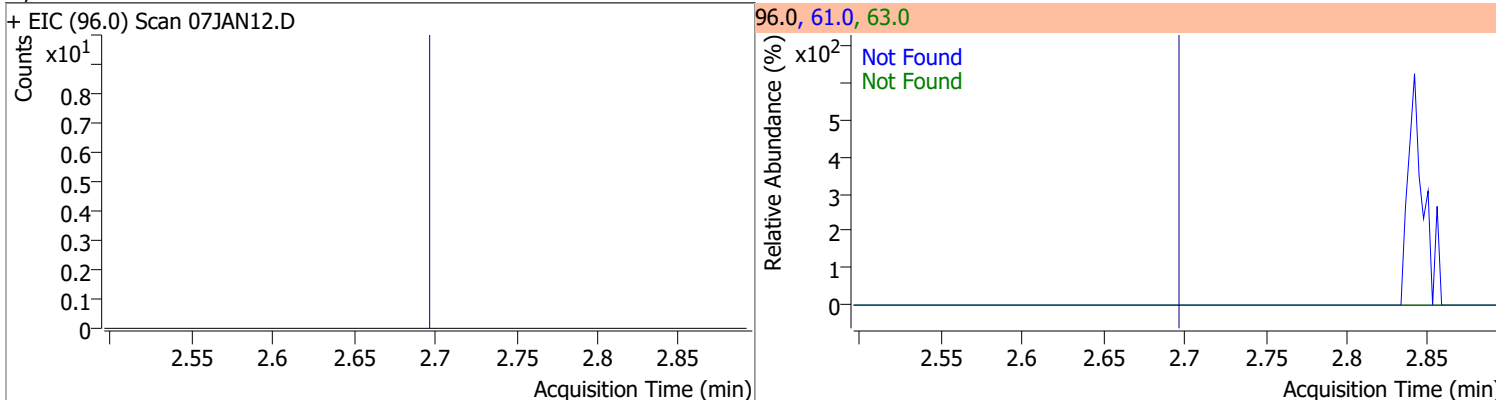

| Compound           | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| Methylene chloride | N.D.  | 3.34   | 84.0 | 66.9      | 86.0 | 44.3      |

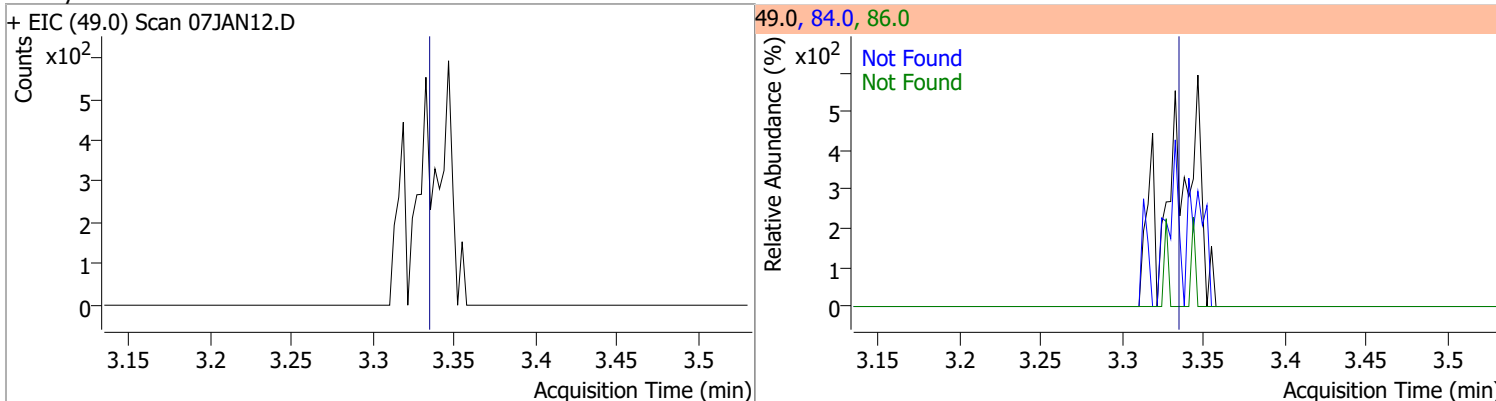


# Quantitation Results Report (QT Reviewed)

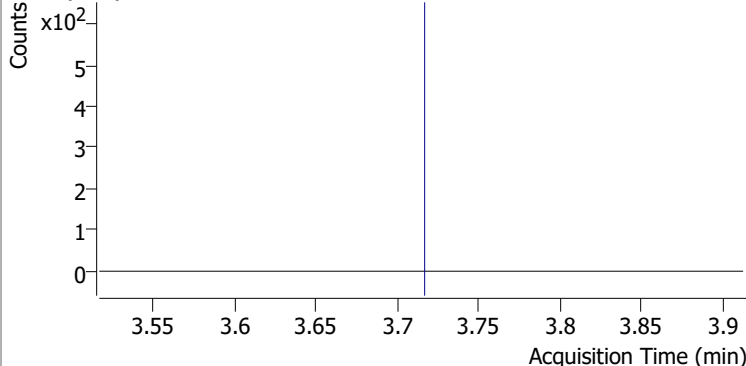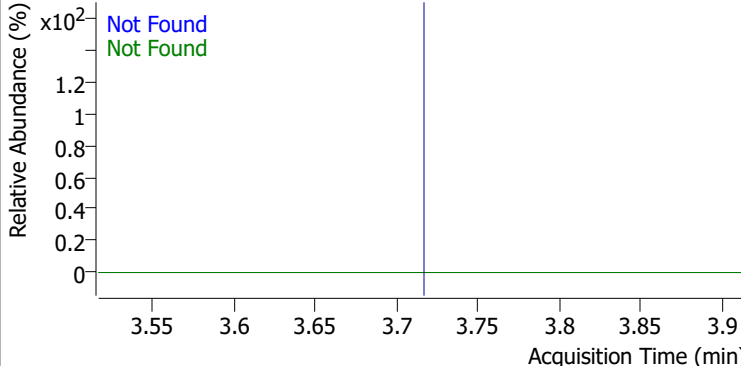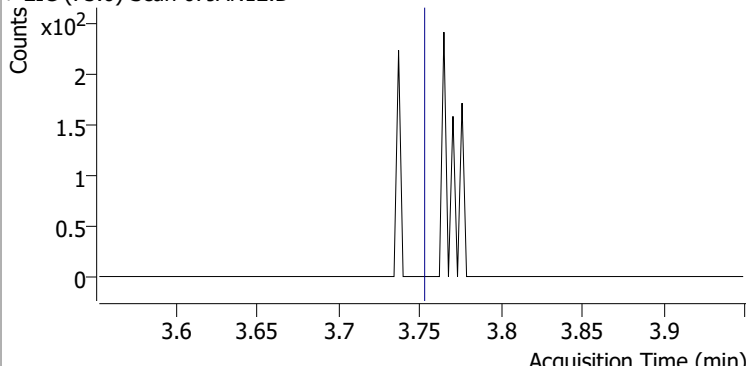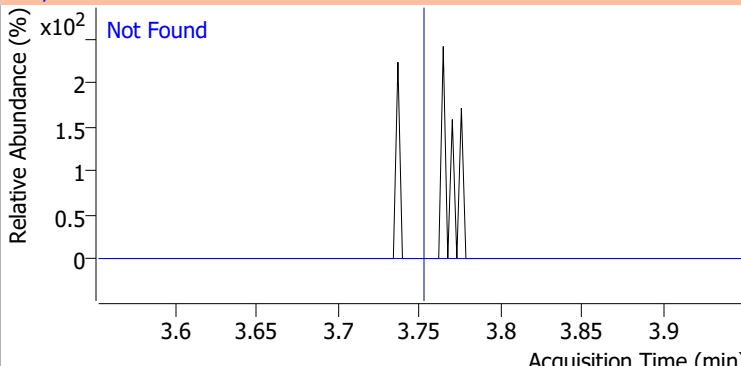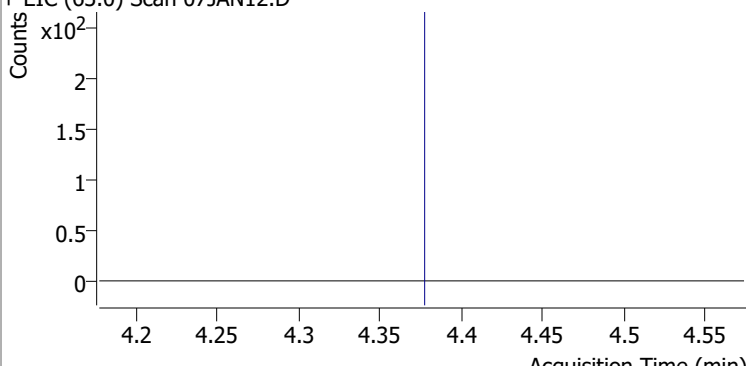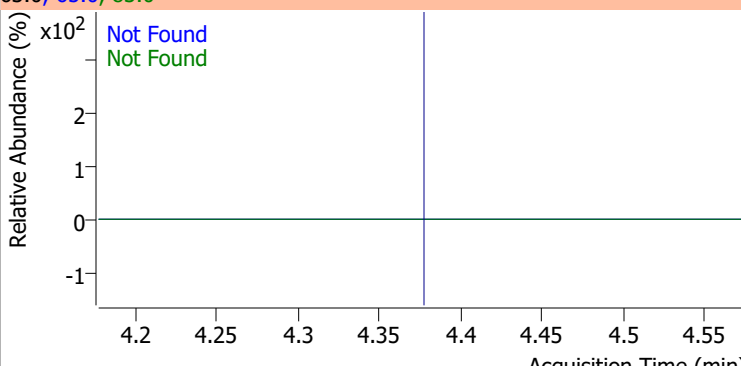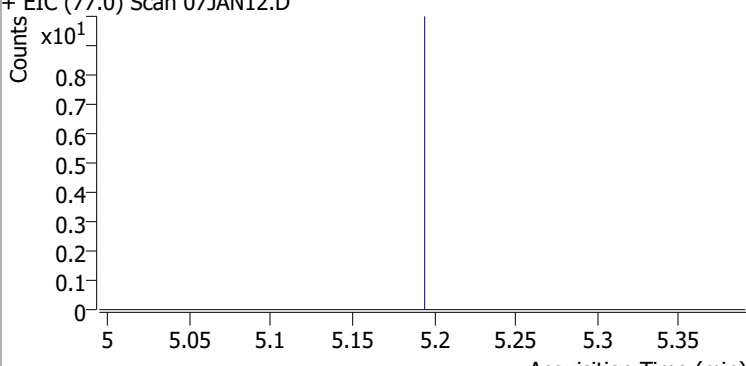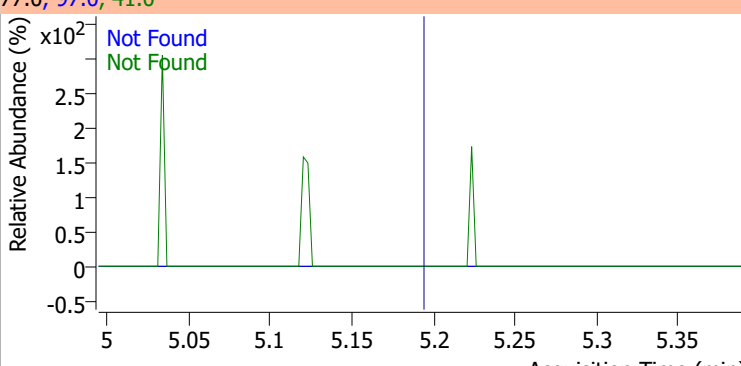
| Compound                                                                           | Conc. | Exp RT | QIon                                                                                 | Exp Ratio | QIon | Exp Ratio |
|------------------------------------------------------------------------------------|-------|--------|--------------------------------------------------------------------------------------|-----------|------|-----------|
| trans-1,2-Dichloroethene                                                           | N.D.  | 3.72   | 61.0                                                                                 | 153.9     | 98.0 | 65.7      |
| + EIC (96.0) Scan 07JAN12.D                                                        |       |        | 96.0, 61.0, 98.0                                                                     |           |      |           |
|    |       |        |    |           |      |           |
| Methyl tert-butyl ether (MTBE)                                                     | N.D.  | 3.75   | 57.0                                                                                 | 24.6      |      |           |
| + EIC (73.0) Scan 07JAN12.D                                                        |       |        | 73.0, 57.0                                                                           |           |      |           |
|   |       |        |   |           |      |           |
| 1,1-Dichloroethane                                                                 | N.D.  | 4.38   | 65.0                                                                                 | 32.1      | 83.0 | 13.7      |
| + EIC (63.0) Scan 07JAN12.D                                                        |       |        | 63.0, 65.0, 83.0                                                                     |           |      |           |
|  |       |        |  |           |      |           |
| 2,2-Dichloropropane                                                                | N.D.  | 5.20   | 41.0                                                                                 | 66.5      | 97.0 | 23.2      |
| + EIC (77.0) Scan 07JAN12.D                                                        |       |        | 77.0, 97.0, 41.0                                                                     |           |      |           |
|  |       |        |  |           |      |           |

# Quantitation Results Report (QT Reviewed)


| Compound               | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|------------------------|-------|--------|------|-----------|------|-----------|
| cis-1,2-Dichloroethene | N.D.  | 5.22   | 61.0 | 167.2     | 98.0 | 67.3      |




| Compound            | Conc.  | RT   | Dev(Min) | Resp.   | QIon | QRatio | Lower | Upper |
|---------------------|--------|------|----------|---------|------|--------|-------|-------|
| Methyl ethyl ketone | 5.0179 | 5.30 | 0.02     | 565 (m) | 72.0 | 22.9   | 0.0   | 51.3  |



| Compound           | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|
| Bromochloromethane | N.D.  | 5.52   | 49.0 | 182.9     |




| Compound   | Conc.  | RT   | Dev(Min) | Resp.    | QIon | QRatio | Lower | Upper |
|------------|--------|------|----------|----------|------|--------|-------|-------|
| Chloroform | 1.0896 | 5.65 | -0.01    | 1655 (m) | 85.0 | 57.2   | 36.0  | 96.0  |






# Quantitation Results Report (QT Reviewed)


| Compound              | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------------|-------|--------|------|-----------|------|-----------|
| 1,1,1-Trichloroethane | N.D.  | 5.83   | 99.0 | 64.7      | 61.0 | 48.1      |




| Compound             | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Dibromofluoromethane | 278.8342 | 5.85 | 0.01     | 209602 | 191.5 | 22.0   | 0.0   | 53.1  |



| Compound             | Conc. | Exp RT | QIon  | Exp Ratio | QIon  | Exp Ratio |
|----------------------|-------|--------|-------|-----------|-------|-----------|
| Carbon tetrachloride | N.D.  | 6.02   | 119.0 | 97.2      | 121.0 | 30.1      |




| Compound            | Conc. | Exp RT | QIon  | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|-------|-----------|------|-----------|
| 1,1-Dichloropropene | N.D.  | 6.04   | 110.0 | 35.9      | 77.0 | 30.1      |




# Quantitation Results Report (QT Reviewed)


| Compound              | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 291.7947 | 6.24 | 0.00     | 94741 | 65.0 | 192.3  | 166.5 | 226.5 |

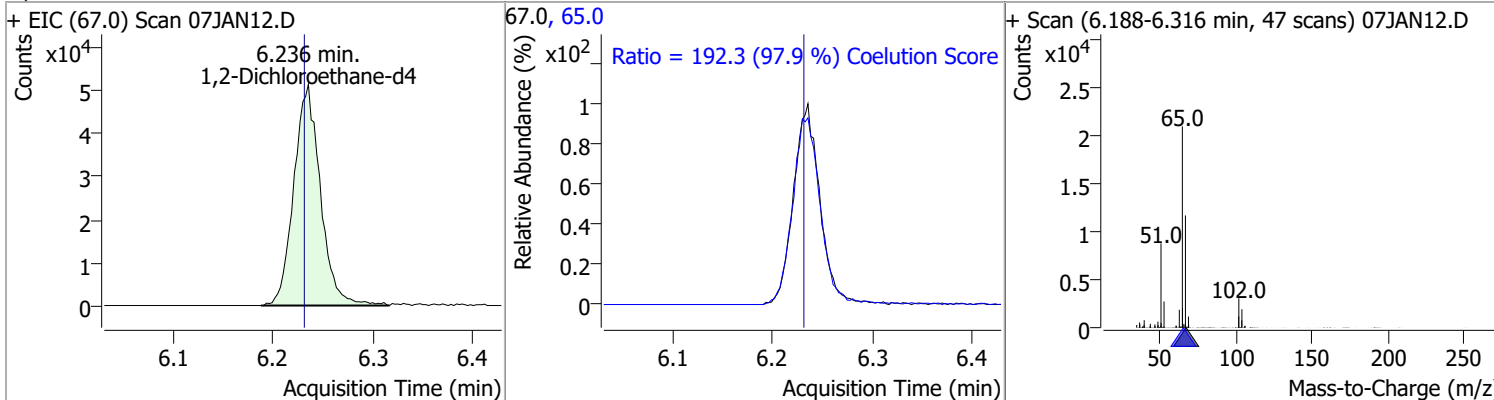


| Compound | Conc.  | RT   | Dev(Min) | Resp.   | QIon | QRatio | Lower | Upper |
|----------|--------|------|----------|---------|------|--------|-------|-------|
| Benzene  | 0.1289 | 6.28 | 0.00     | 409 (m) | 77.0 | 10.6   | 0.0   | 53.5  |

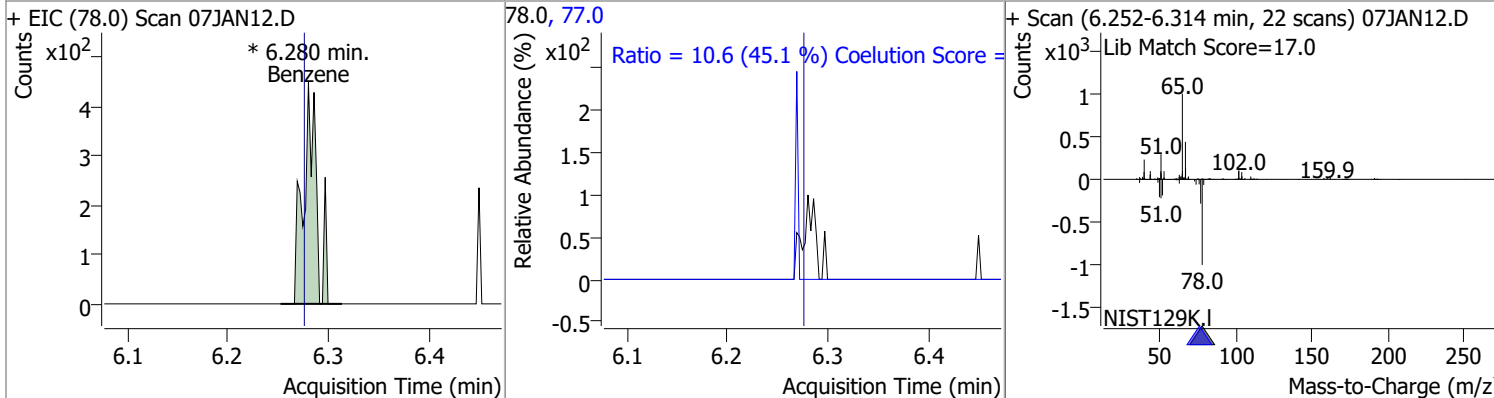


| Compound           | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,2-Dichloroethane | N.D.  | 6.32   | 64.0 | 29.9      | 98.0 | 7.6       |

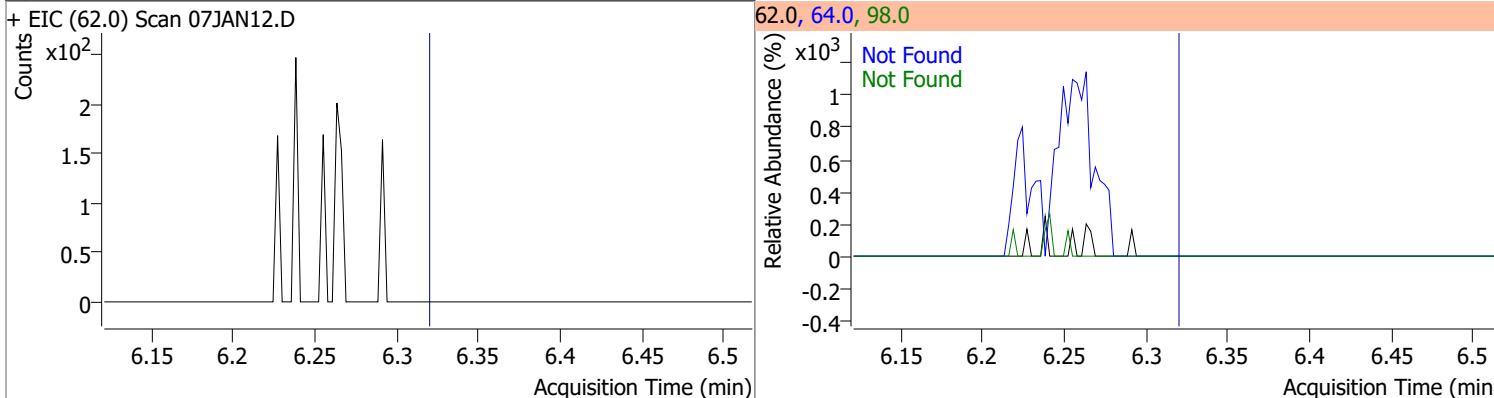


| Compound        | Conc. | Exp RT | QIon  | Exp Ratio | QIon | Exp Ratio |
|-----------------|-------|--------|-------|-----------|------|-----------|
| Trichloroethene | N.D.  | 7.03   | 130.0 | 101.5     | 97.0 | 64.1      |

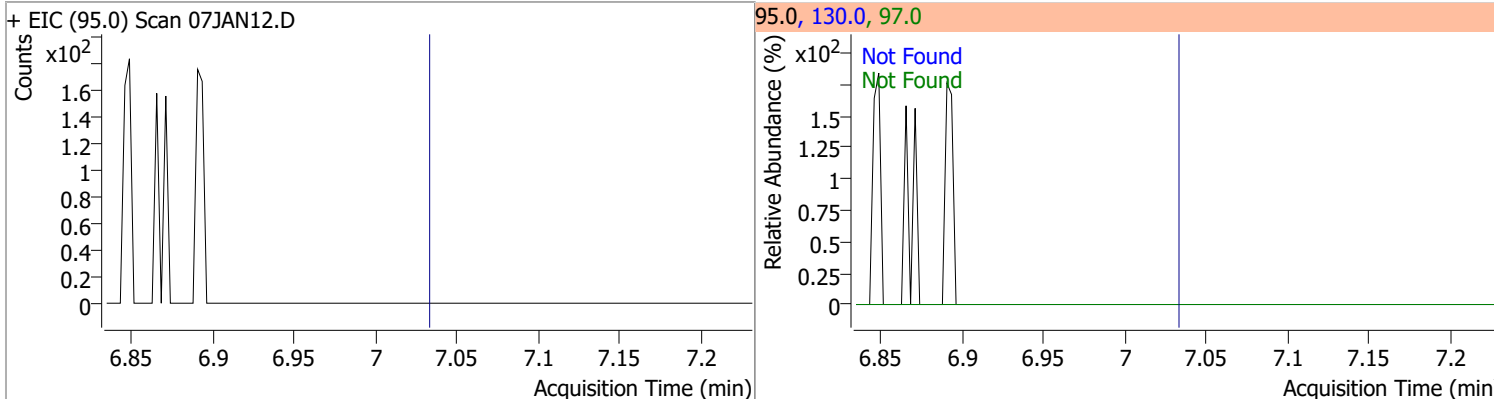


# Quantitation Results Report (QT Reviewed)

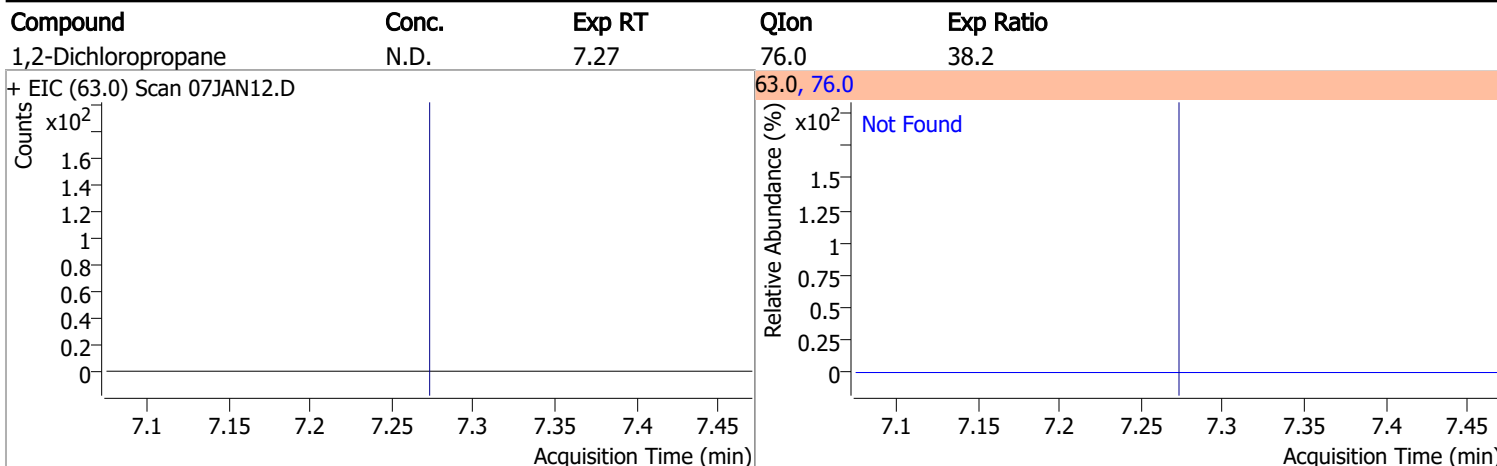


| Compound       | Conc.  | RT   | Dev(Min) | Resp.   | QIon  | QRatio | Lower | Upper |
|----------------|--------|------|----------|---------|-------|--------|-------|-------|
| Dibromomethane | 0.3122 | 7.40 | 0.00     | 111 (m) | 173.5 | 121.7  | 83.7  | 143.7 |
|                |        |      |          |         | 95.0  | 60.7   | 52.2  | 112.2 |

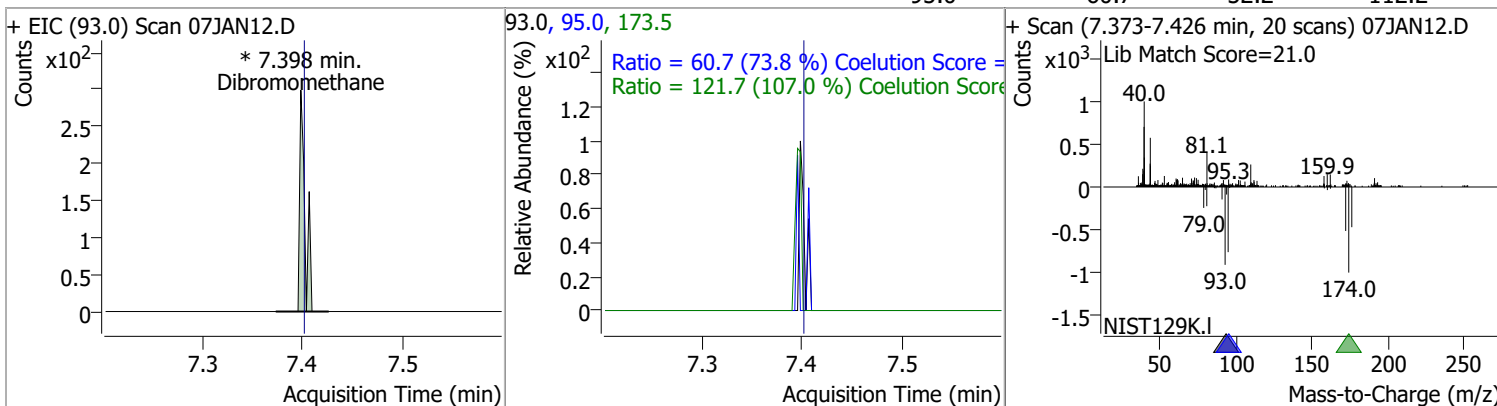

| Compound             | Conc.  | RT   | Dev(Min) | Resp.   | QIon  | QRatio | Lower | Upper |
|----------------------|--------|------|----------|---------|-------|--------|-------|-------|
| Bromodichloromethane | 0.6660 | 7.59 | 0.01     | 654 (m) | 85.0  | 59.7   | 34.5  | 94.5  |
|                      |        |      |          |         | 127.0 | 5.2    | 0.0   | 39.6  |

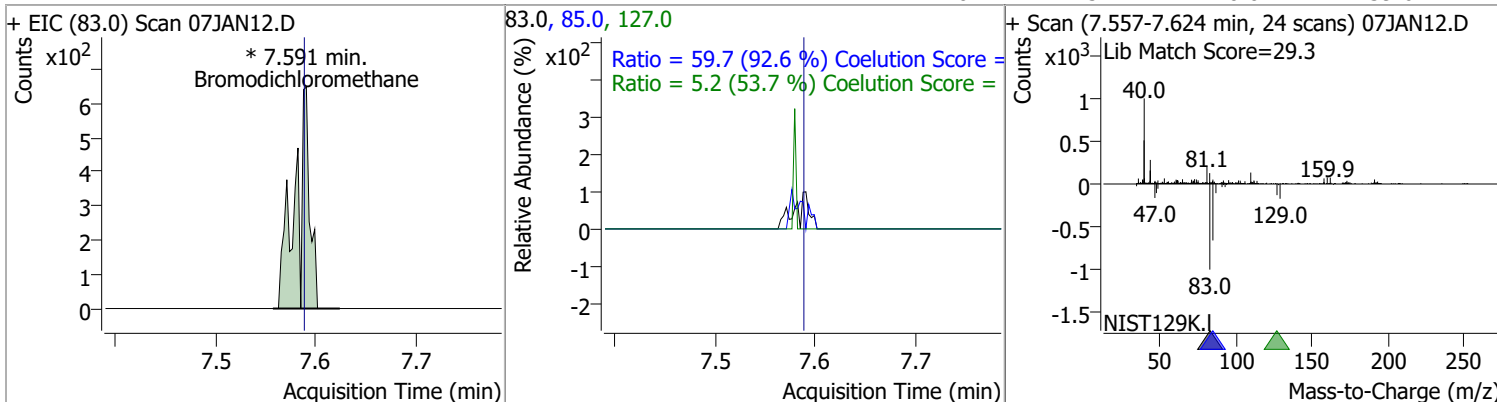


| Compound                | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-------------------------|-------|--------|------|-----------|------|-----------|
| cis-1,3-Dichloropropene | N.D.  | 8.06   | 39.0 | 53.3      | 77.0 | 31.0      |

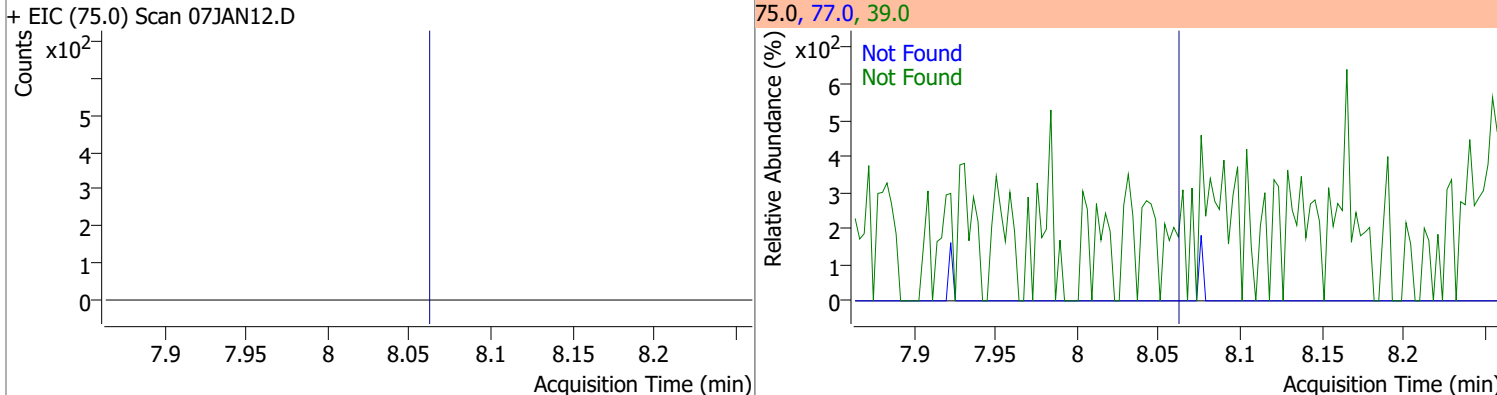


# Quantitation Results Report (QT Reviewed)


| Compound   | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 261.6097 | 8.32 | 0.00     | 800313 | 100.0 | 63.4   | 34.4  | 94.4  |
|            |          |      |          |        | 99.0  | 10.0   | 0.0   | 39.6  |

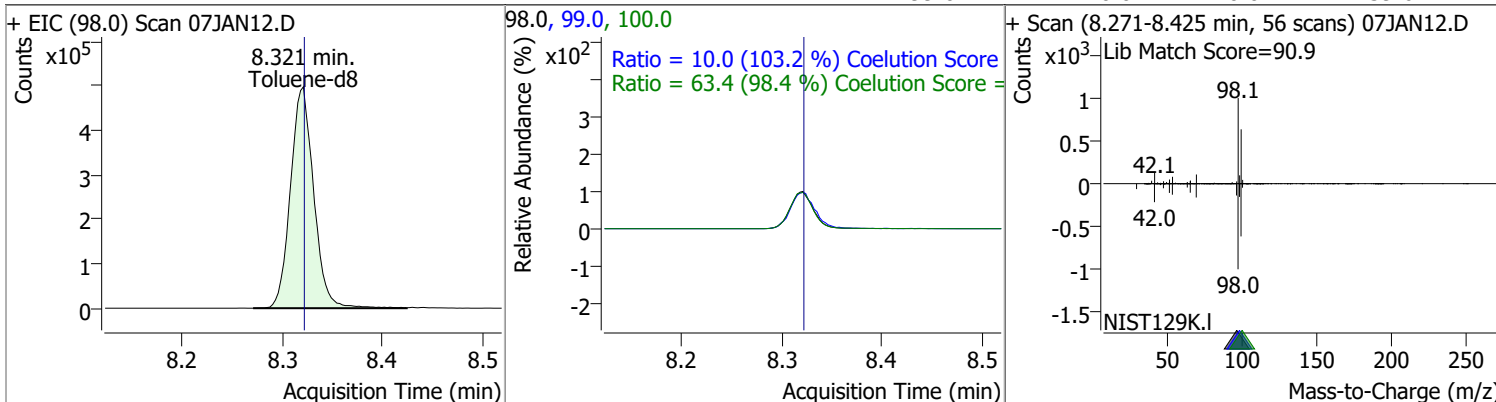


| Compound | Conc.  | RT   | Dev(Min) | Resp.   | QIon | QRatio | Lower | Upper |
|----------|--------|------|----------|---------|------|--------|-------|-------|
| Toluene  | 0.2388 | 8.39 | 0.00     | 493 (m) | 91.0 | 179.9  | 145.8 | 205.8 |

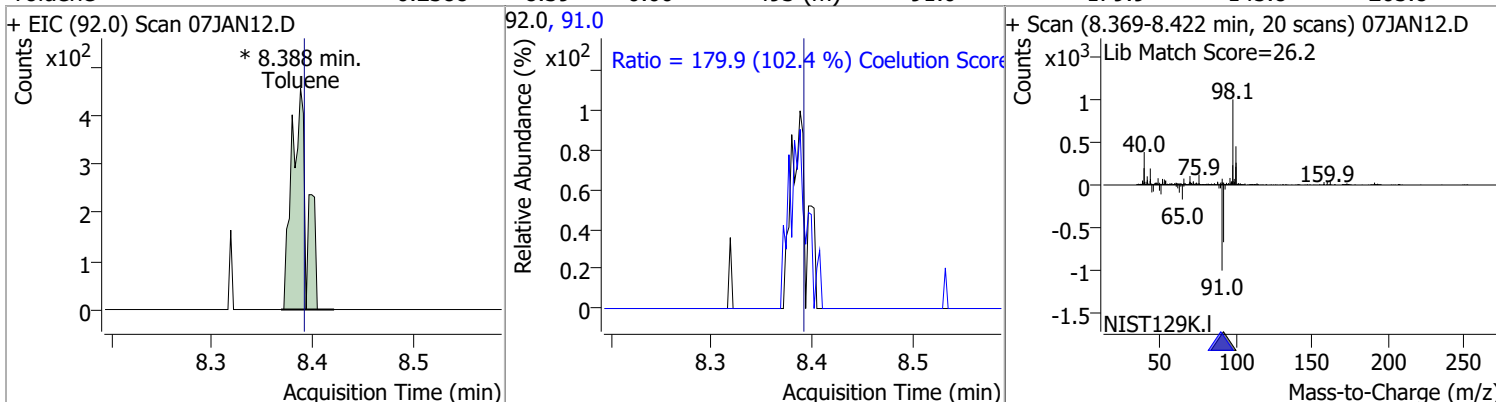

| Compound                  | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,3-Dichloropropene | N.D.  | 8.64   | 39.0 | 53.4      | 77.0 | 32.4      |

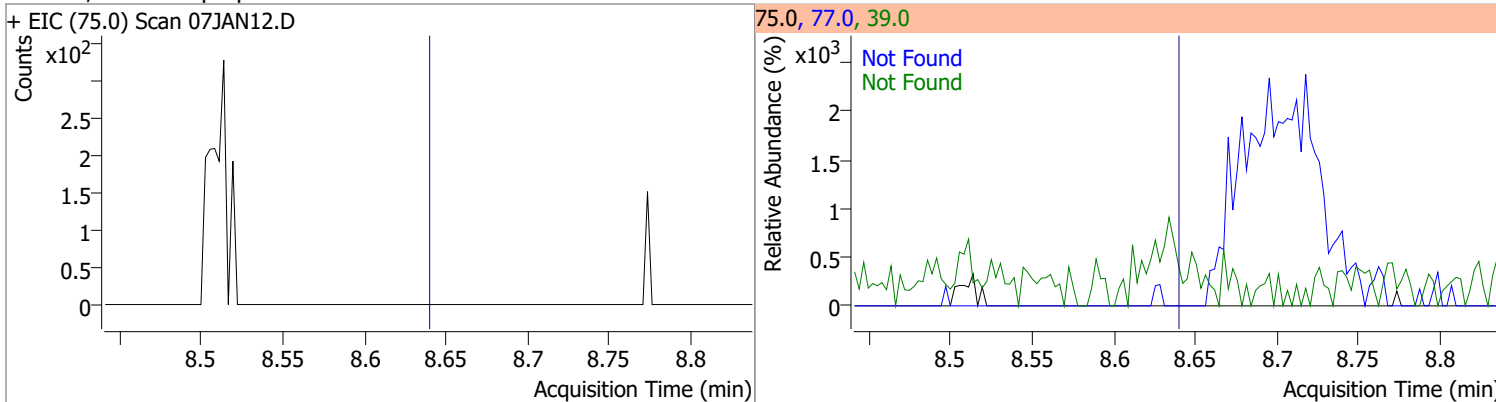


| Compound              | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------------|-------|--------|------|-----------|------|-----------|
| 1,1,2-Trichloroethane | N.D.  | 8.82   | 97.0 | 114.6     | 85.0 | 67.6      |

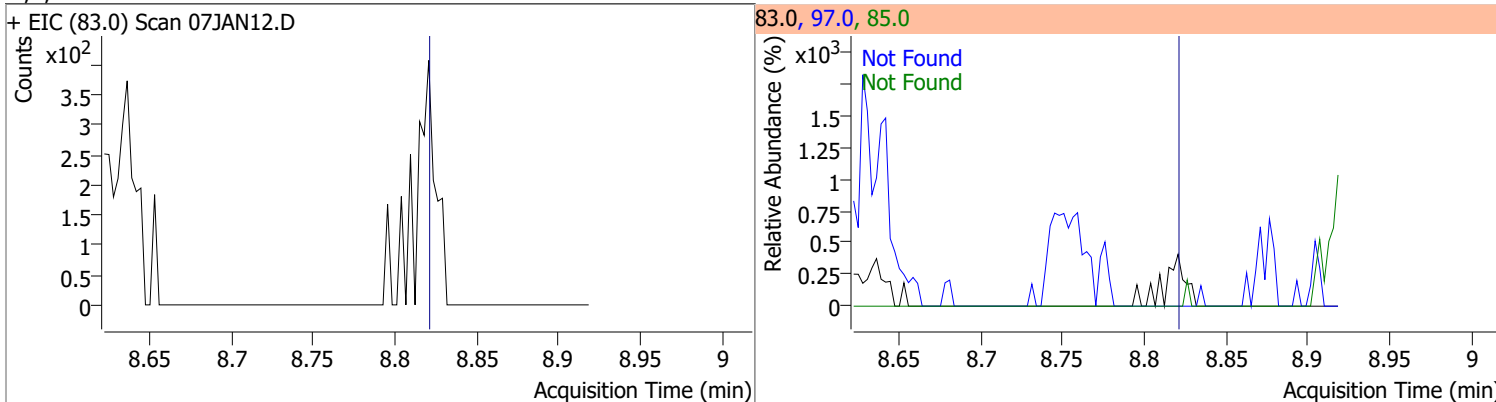


# Quantitation Results Report (QT Reviewed)


| Compound          | Conc. | Exp RT | QIon  | Exp Ratio | QIon  | Exp Ratio |
|-------------------|-------|--------|-------|-----------|-------|-----------|
| Tetrachloroethene | N.D.  | 8.94   | 165.8 | 128.6     | 129.0 | 91.5      |




| Compound            | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| 1,3-Dichloropropane | N.D.  | 8.98   | 78.0 | 32.9      |







| Compound             | Conc.  | RT   | Dev(Min) | Resp.    | QIon  | QRatio | Lower | Upper |
|----------------------|--------|------|----------|----------|-------|--------|-------|-------|
| Chlorodibromomethane | 2.4889 | 9.21 | 0.01     | 1602 (m) | 127.0 | 60.7   | 48.0  | 108.0 |







| Compound          | Conc. | Exp RT | QIon  | Exp Ratio |
|-------------------|-------|--------|-------|-----------|
| 1,2-Dibromoethane | N.D.  | 9.31   | 109.0 | 94.5      |



# Quantitation Results Report (QT Reviewed)




# Quantitation Results Report (QT Reviewed)

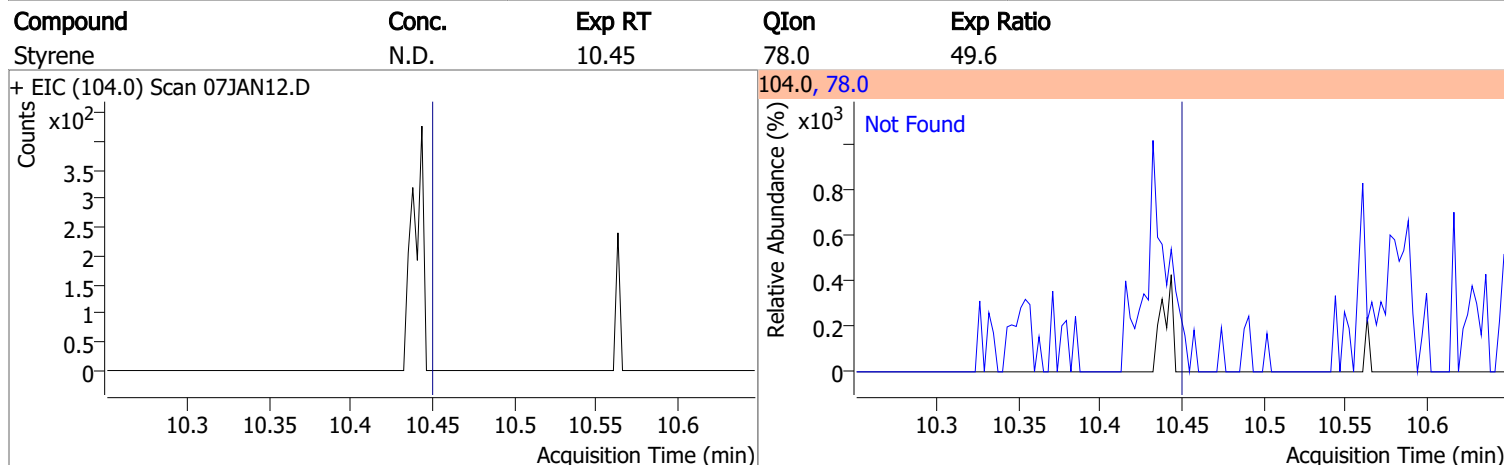


# Quantitation Results Report (QT Reviewed)


| Compound     | Conc. | Exp RT | QIon | Exp Ratio | QIon  | Exp Ratio |
|--------------|-------|--------|------|-----------|-------|-----------|
| Bromobenzene | N.D.  | 11.09  | 77.0 | 145.7     | 158.0 | 96.5      |




| Compound                  | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|-------|----|----------|-------|------|--------|-------|-------|
| 1,1,2,2-Tetrachloroethane | 0     | 0  | 0        | 0     | 85.0 |        | 36.2  | 96.2  |



| Compound               | Conc. | RT | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|------------------------|-------|----|----------|-------|-------|--------|-------|-------|
| 1,2,3-Trichloropropane | 0     | 0  | 0        | 0     | 112.0 |        | 33.5  | 93.5  |





| Compound        | Conc. | Exp RT | QIon | Exp Ratio |
|-----------------|-------|--------|------|-----------|
| 2-Chlorotoluene | N.D.  | 11.29  | 91.0 | 282.3     |







# Quantitation Results Report (QT Reviewed)



| Compound        | Conc. | RT | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|-----------------|-------|----|----------|-------|-------|--------|-------|-------|
| 4-Chlorotoluene | 0     | 0  |          | 0     | 126.0 |        | 1.7   | 61.7  |





| Compound            | Conc. | Exp RT | QIon  | Exp Ratio | QIon  | Exp Ratio |
|---------------------|-------|--------|-------|-----------|-------|-----------|
| 1,3-Dichlorobenzene | N.D.  | 12.03  | 148.0 | 63.6      | 111.0 | 39.8      |



| Compound            | Conc. | Exp RT | QIon  | Exp Ratio | QIon  | Exp Ratio |
|---------------------|-------|--------|-------|-----------|-------|-----------|
| 1,4-Dichlorobenzene | N.D.  | 12.13  | 148.0 | 63.1      | 111.0 | 39.1      |




| Compound            | Conc. | Exp RT | QIon  | Exp Ratio | QIon  | Exp Ratio |
|---------------------|-------|--------|-------|-----------|-------|-----------|
| 1,2-Dichlorobenzene | N.D.  | 12.49  | 148.0 | 63.9      | 111.0 | 41.0      |



# Quantitation Results Report (QT Reviewed)

|                |                                     |                   |                       |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File      | 07JAN14.D                           | Operator          | MSC                   |
| Acq. Method    | 5975CACQF.M                         | Acq. Date-Time    | 1/7/2022 3:35:59 PM   |
| Sample Name    | B22010214-001F                      | Instrument        | VOA5975C              |
| Vial           | 14                                  | Multiplier        | 1.00                  |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m  | Comment           |                       |
| Tune File      | BFB_Atune3.u                        | Tune Date         | 10/11/2021 4:02:00 PM |
| Batch Name     | VG010722_8260B.batch.bin            | Last Calib Update | 3/2/2022 10:41:44 AM  |
| Ref Library    | \\MASSHUNTER\Org\Library\NIST129K.I |                   |                       |

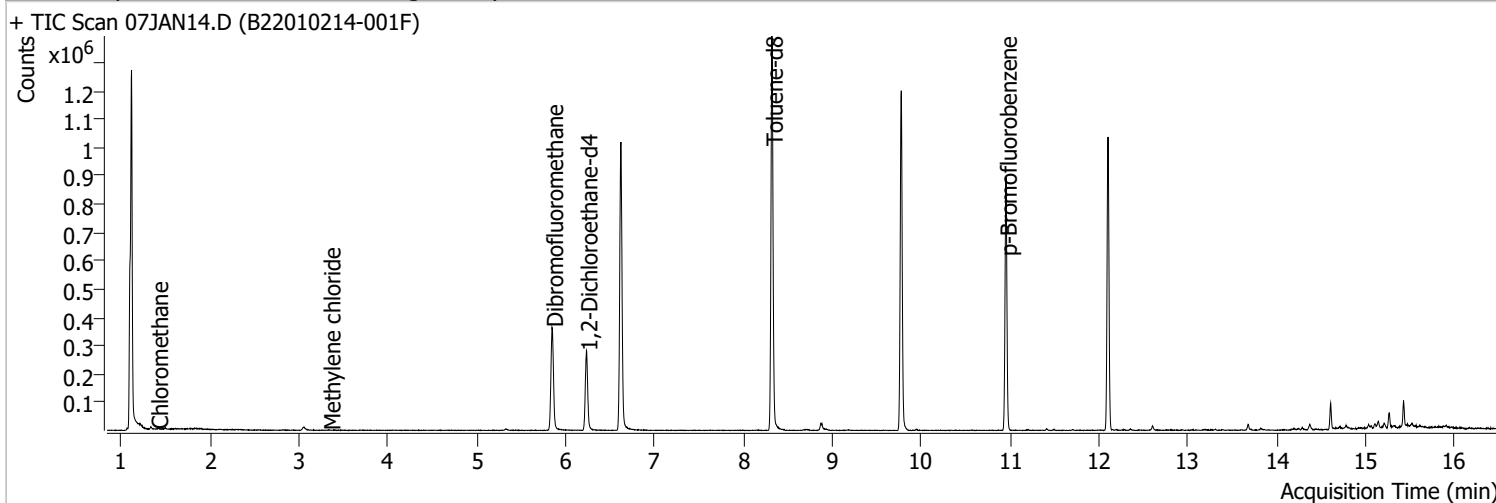

| Compound | RT | QIon | Resp. | Conc. | Units | Dev(Min) |
|----------|----|------|-------|-------|-------|----------|
|----------|----|------|-------|-------|-------|----------|

**Internal Standards**

|                          |        |       |        |          |    |        |
|--------------------------|--------|-------|--------|----------|----|--------|
| M Fluorobenzene          | 6.620  | 96.0  | 850985 | 250.0000 | ng | -0.003 |
| M Chlorobenzene-d5       | 9.772  | 82.0  | 331791 | 250.0000 | ng | 0.000  |
| M 1,4-Dichlorobenzene-d4 | 12.100 | 152.0 | 251886 | 250.0000 | ng | 0.000  |

**System Monitoring Compounds**

|                         |                      |       |        |                    |    |        |
|-------------------------|----------------------|-------|--------|--------------------|----|--------|
| S Dibromofluoromethane  | 5.845                | 113.0 | 224189 | 279.6371           | ng | 0.000  |
| Spiked Amount: 250.000  | Range: 80.0 - 119.0% |       |        | Recovery = 111.85% |    |        |
| S 1,2-Dichloroethane-d4 | 6.233                | 67.0  | 99414  | 287.0891           | ng | 0.000  |
| Spiked Amount: 250.000  | Range: 81.0 - 118.0% |       |        | Recovery = 114.84% |    |        |
| S Toluene-d8            | 8.319                | 98.0  | 856527 | 267.8901           | ng | 0.000  |
| Spiked Amount: 250.000  | Range: 89.0 - 112.0% |       |        | Recovery = 107.16% |    |        |
| S p-Bromofluorobenzene  | 10.951               | 95.0  | 255176 | 276.5273           | ng | -0.003 |
| Spiked Amount: 250.000  | Range: 85.0 - 114.0% |       |        | Recovery = 110.61% |    |        |

**Target Compounds**

| Compound                         | RT    | QIon | Resp. | Conc.  | Units | QValue |
|----------------------------------|-------|------|-------|--------|-------|--------|
| T Dichlorodifluoromethane        | 0.000 |      | 0     | N.D.   |       |        |
| T Chloromethane                  | 1.406 | 50.0 | 2350  | 1.7362 | ng    | 98     |
| T Vinyl chloride                 | 0.000 |      | 0     | N.D.   |       |        |
| T Bromomethane                   | 0.000 |      | 0     | N.D.   |       |        |
| T Chloroethane                   | 0.000 |      | 0     | N.D.   |       |        |
| T Trichlorofluoromethane         | 0.000 |      | 0     | N.D.   |       |        |
| T 1,1-Dichloroethene             | 0.000 |      | 0     | N.D.   |       |        |
| T Methylene chloride             | 3.344 | 49.0 | 885   | 0.7000 | ng    | 82     |
| T trans-1,2-Dichloroethene       | 0.000 |      | 0     | N.D.   |       |        |
| T Methyl tert-butyl ether (MTBE) | 0.000 |      | 0     | N.D.   |       |        |
| T 1,1-Dichloroethane             | 0.000 |      | 0     | N.D.   |       |        |
| T 2,2-Dichloropropane            | 0.000 |      | 0     | N.D.   |       |        |
| T cis-1,2-Dichloroethene         | 0.000 |      | 0     | N.D.   |       |        |
| T Methyl ethyl ketone            | 0.000 |      | 0     | N.D.   |       |        |
| T Bromochloromethane             | 0.000 |      | 0     | N.D.   |       |        |
| T Chloroform                     | 0.000 |      | 0     | N.D.   |       |        |


# Quantitation Results Report (QT Reviewed)

| Compound                    | RT    | QIon | Resp. | Conc. | Units | Dev(Min) |
|-----------------------------|-------|------|-------|-------|-------|----------|
| T 1,1,1-Trichloroethane     | 0.000 |      | 0     | N.D.  |       |          |
| T Carbon tetrachloride      | 0.000 |      | 0     | N.D.  |       |          |
| T 1,1-Dichloropropene       | 0.000 |      | 0     | N.D.  |       |          |
| T Benzene                   | 0.000 |      | 0     | N.D.  |       |          |
| T 1,2-Dichloroethane        | 0.000 |      | 0     | N.D.  |       |          |
| T Trichloroethene           | 0.000 |      | 0     | N.D.  |       |          |
| T 1,2-Dichloropropane       | 0.000 |      | 0     | N.D.  |       |          |
| T Dibromomethane            | 0.000 |      | 0     | N.D.  |       |          |
| T Bromodichloromethane      | 0.000 |      | 0     | N.D.  |       |          |
| T cis-1,3-Dichloropropene   | 0.000 |      | 0     | N.D.  |       |          |
| T Toluene                   | 8.377 | 92.0 | 0     |       | ng md | 1        |
| T trans-1,3-Dichloropropene | 0.000 |      | 0     | N.D.  |       |          |
| T 1,1,2-Trichloroethane     | 0.000 |      | 0     | N.D.  |       |          |
| T Tetrachloroethene         | 0.000 |      | 0     | N.D.  |       |          |
| T 1,3-Dichloropropane       | 0.000 |      | 0     | N.D.  |       |          |
| T Chlorodibromomethane      | 0.000 |      | 0     | N.D.  |       |          |
| T 1,2-Dibromoethane         | 0.000 |      | 0     | N.D.  |       |          |
| T Chlorobenzene             | 0.000 |      | 0     | N.D.  |       |          |
| T 1,1,1,2-Tetrachloroethane | 0.000 |      | 0     | N.D.  |       |          |
| T Ethylbenzene              | 0.000 |      | 0     | N.D.  |       |          |
| T m+p-Xylenes               | 0.000 |      | 0     | N.D.  |       |          |
| T o-Xylene                  | 0.000 |      | 0     | N.D.  |       |          |
| T Styrene                   | 0.000 |      | 0     | N.D.  |       |          |
| T Bromoform                 | 0.000 |      | 0     | N.D.  |       |          |
| T Bromobenzene              | 0.000 |      | 0     | N.D.  |       |          |
| T 1,1,2,2-Tetrachloroethane | 0.000 |      | 0     | N.D.  |       |          |
| T 1,2,3-Trichloropropane    | 0.000 |      | 0     | N.D.  |       |          |
| T 2-Chlorotoluene           | 0.000 |      | 0     | N.D.  |       |          |
| T 4-Chlorotoluene           | 0.000 |      | 0     | N.D.  |       |          |
| T 1,3-Dichlorobenzene       | 0.000 |      | 0     | N.D.  |       |          |
| T 1,4-Dichlorobenzene       | 0.000 |      | 0     | N.D.  |       |          |
| T 1,2-Dichlorobenzene       | 0.000 |      | 0     | N.D.  |       |          |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (\*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

# Quantitation Results Report (QT Reviewed)


| Compound                | Conc. | Exp RT | QIon | Exp Ratio |
|-------------------------|-------|--------|------|-----------|
| Dichlorodifluoromethane | N.D.  | 1.24   | 87.0 | 32.3      |




| Compound      | Conc.  | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------|--------|------|----------|-------|------|--------|-------|-------|
| Chloromethane | 1.7362 | 1.41 | 0.00     | 2350  | 52.0 | 30.9   | 2.1   | 62.1  |



| Compound       | Conc. | Exp RT | QIon | Exp Ratio |
|----------------|-------|--------|------|-----------|
| Vinyl chloride | N.D.  | 1.50   | 64.0 | 29.9      |




| Compound     | Conc. | Exp RT | QIon | Exp Ratio |
|--------------|-------|--------|------|-----------|
| Bromomethane | N.D.  | 1.80   | 94.0 | 104.6     |




# Quantitation Results Report (QT Reviewed)


| Compound     | Conc. | Exp RT | QIon | Exp Ratio |
|--------------|-------|--------|------|-----------|
| Chloroethane | N.D.  | 1.89   | 66.0 | 30.1      |

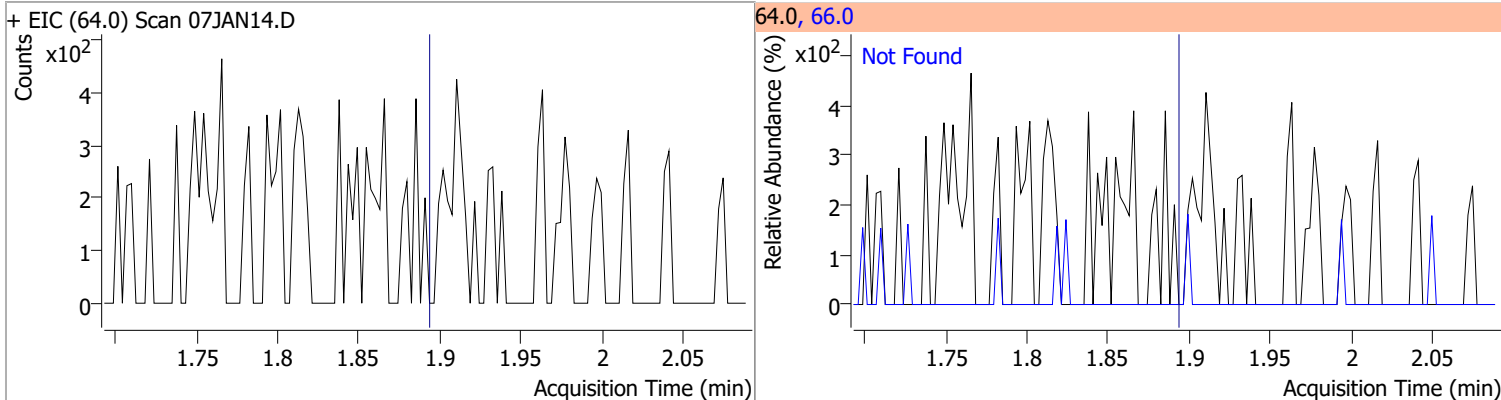


| Compound               | Conc. | Exp RT | QIon  | Exp Ratio |
|------------------------|-------|--------|-------|-----------|
| Trichlorofluoromethane | N.D.  | 2.14   | 103.0 | 64.2      |

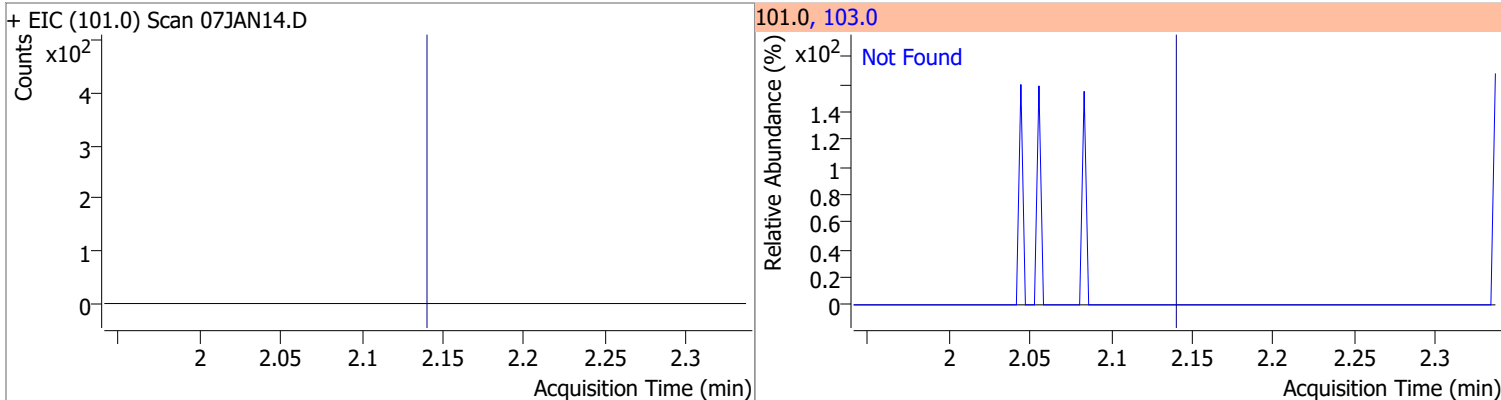

| Compound           | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethene | N.D.  | 2.70   | 61.0 | 180.3     | 63.0 | 56.7      |

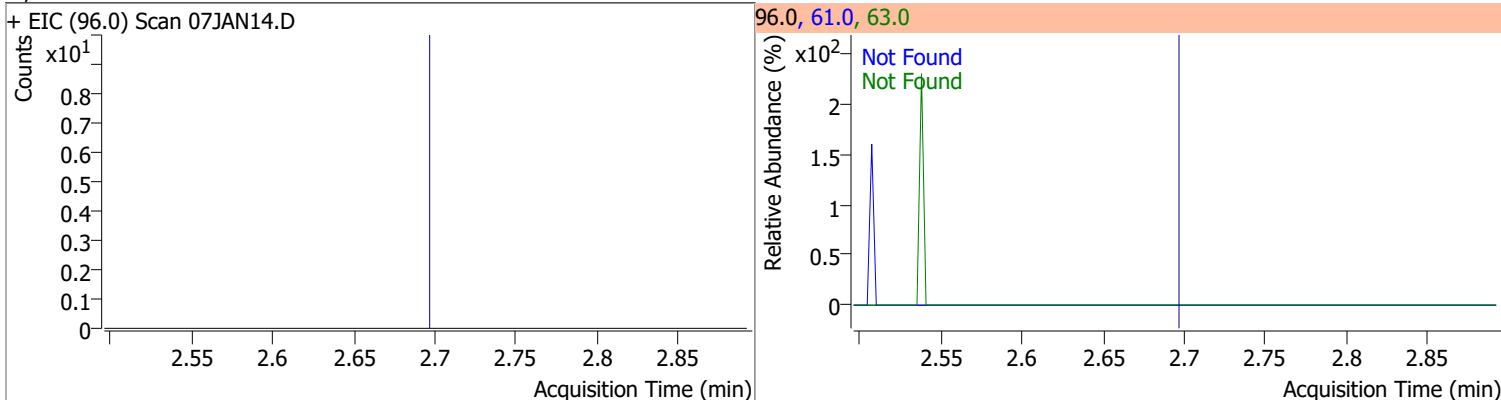


| Compound           | Conc.  | RT   | Dev(Min) | Resp.   | QIon | QRatio | Lower | Upper |
|--------------------|--------|------|----------|---------|------|--------|-------|-------|
| Methylene chloride | 0.7000 | 3.34 | 0.01     | 885 (m) | 84.0 | 50.6   | 36.9  | 96.9  |
|                    |        |      |          |         | 86.0 | 35.4   | 14.3  | 74.3  |

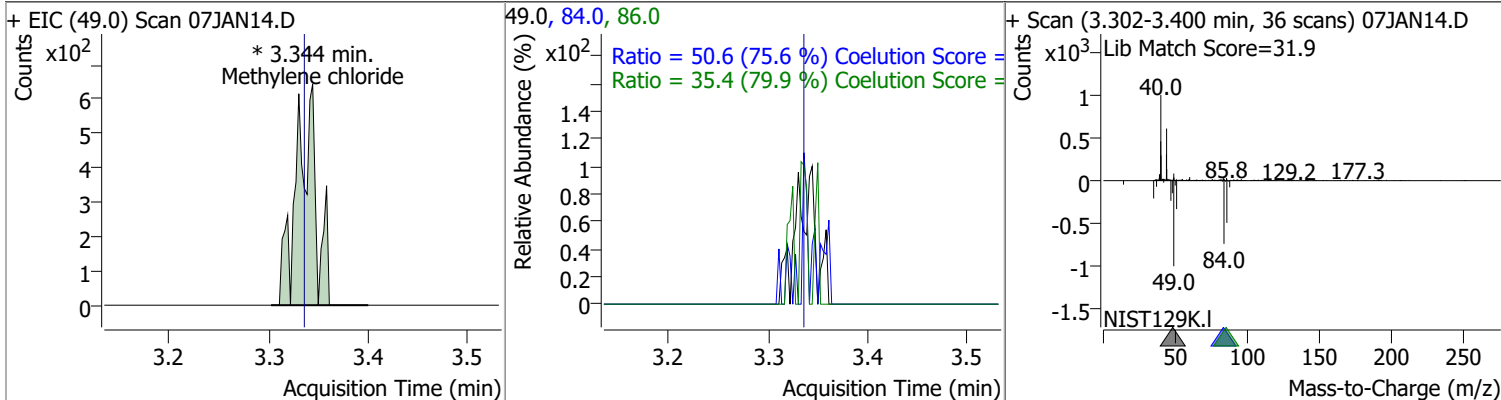


# Quantitation Results Report (QT Reviewed)


| Compound                 | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,2-Dichloroethene | N.D.  | 3.72   | 61.0 | 153.9     | 98.0 | 65.7      |




| Compound                       | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------------------|-------|--------|------|-----------|
| Methyl tert-butyl ether (MTBE) | N.D.  | 3.75   | 57.0 | 24.6      |



| Compound           | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethane | N.D.  | 4.38   | 65.0 | 32.1      | 83.0 | 13.7      |




| Compound            | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|------|-----------|
| 2,2-Dichloropropane | N.D.  | 5.20   | 41.0 | 66.5      | 97.0 | 23.2      |




# Quantitation Results Report (QT Reviewed)


| Compound               | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|------------------------|-------|--------|------|-----------|------|-----------|
| cis-1,2-Dichloroethene | N.D.  | 5.22   | 61.0 | 167.2     | 98.0 | 67.3      |




| Compound            | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| Methyl ethyl ketone | N.D.  | 5.28   | 72.0 | 21.3      |







| Compound           | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|
| Bromochloromethane | N.D.  | 5.52   | 49.0 | 182.9     |



| Compound   | Conc. | Exp RT | QIon | Exp Ratio |
|------------|-------|--------|------|-----------|
| Chloroform | N.D.  | 5.65   | 85.0 | 66.0      |




# Quantitation Results Report (QT Reviewed)

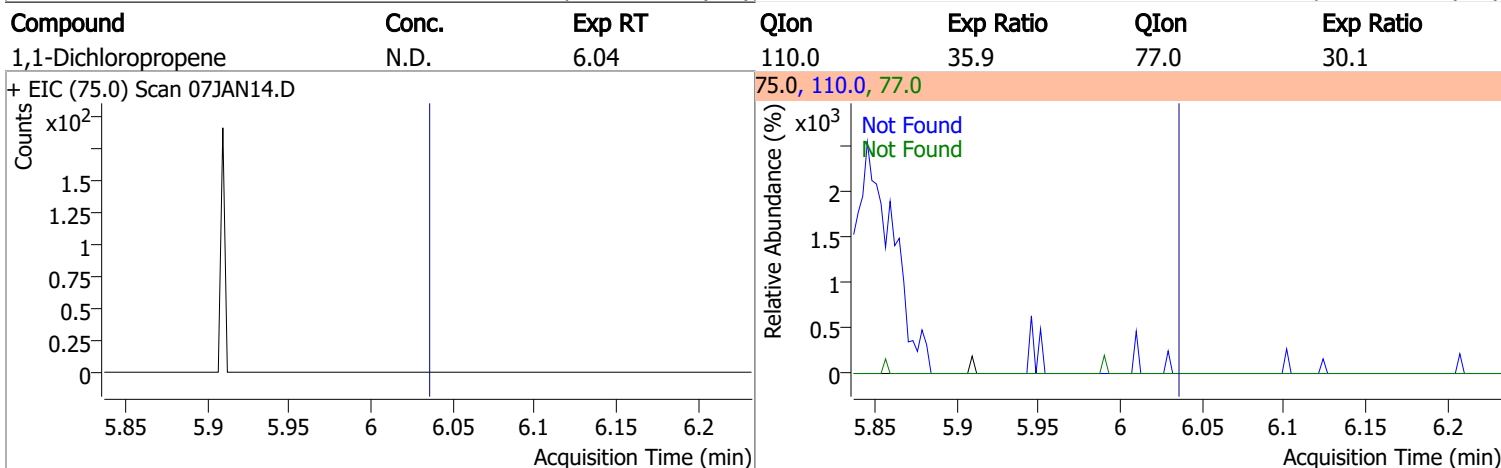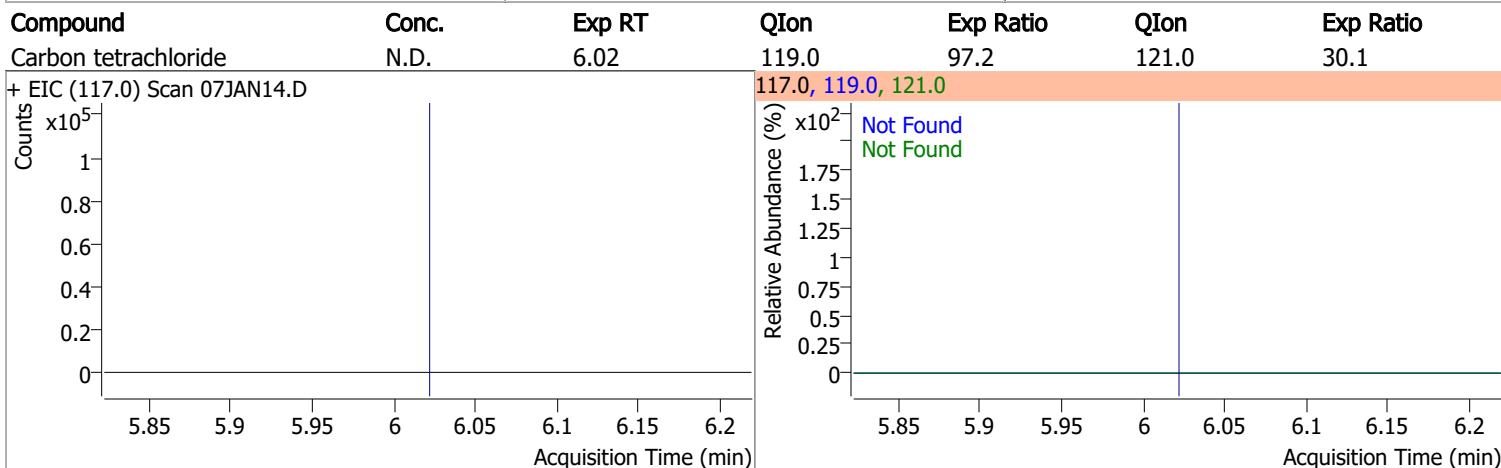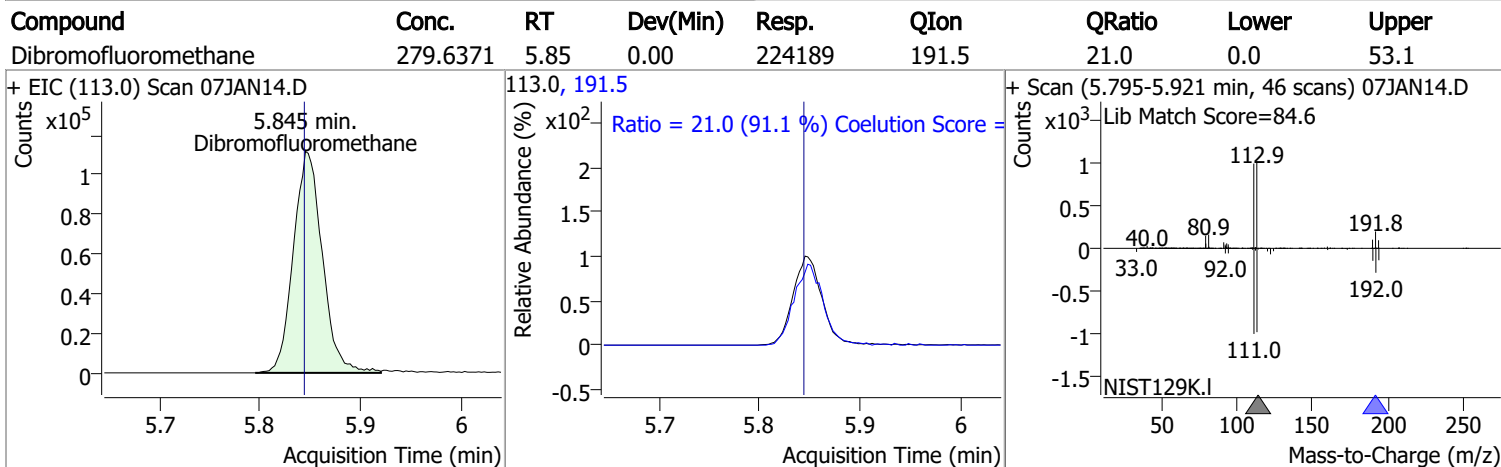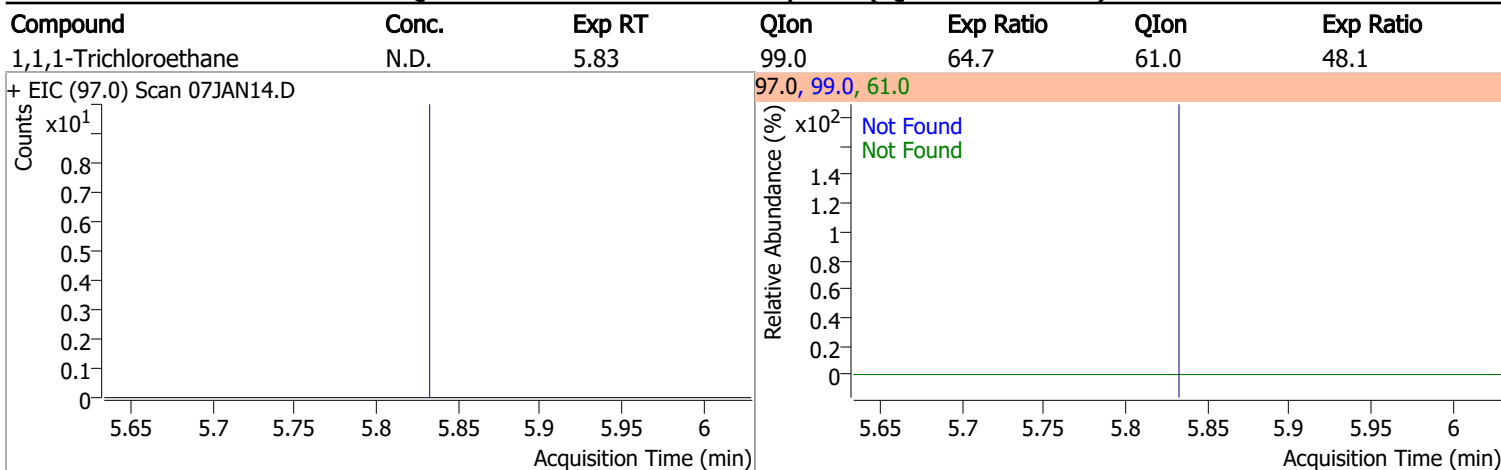




# Quantitation Results Report (QT Reviewed)


| Compound              | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 287.0891 | 6.23 | 0.00     | 99414 | 65.0 | 197.1  | 166.5 | 226.5 |

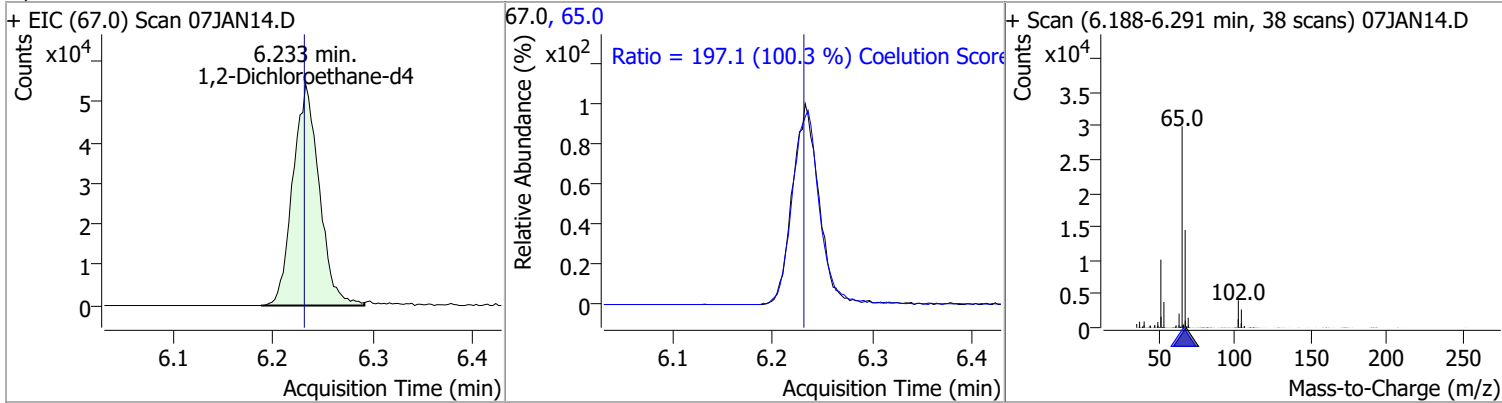


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------|-------|--------|------|-----------|
| Benzene  | N.D.  | 6.28   | 77.0 | 23.5      |

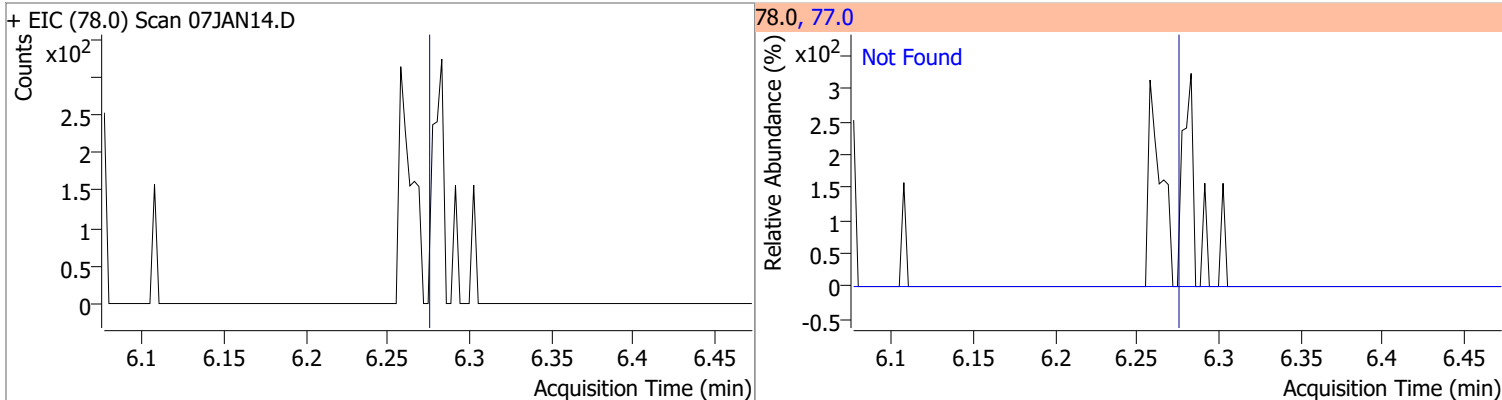





| Compound           | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,2-Dichloroethane | N.D.  | 6.32   | 64.0 | 29.9      | 98.0 | 7.6       |

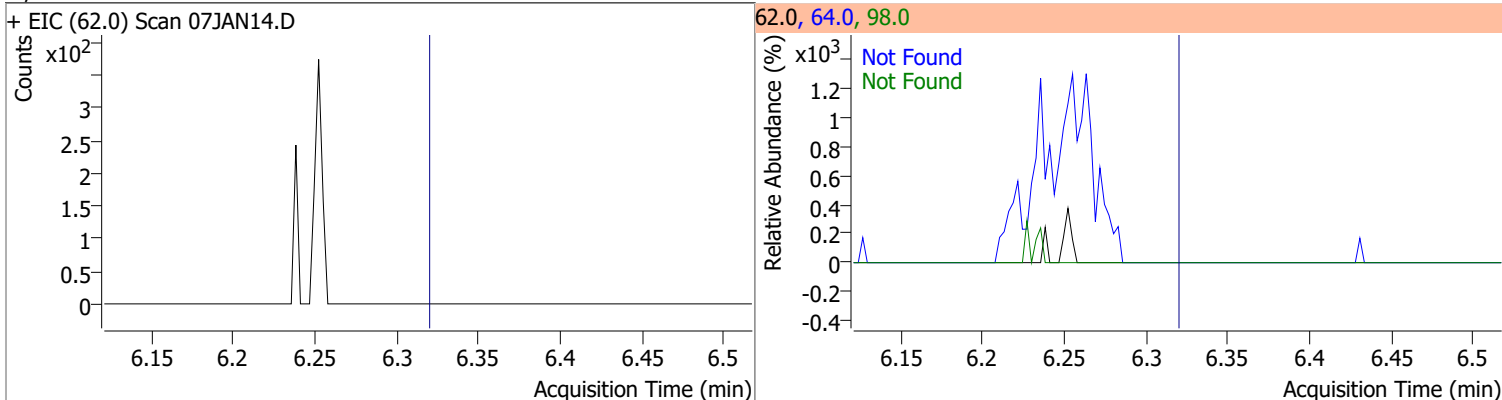

| Compound        | Conc. | Exp RT | QIon  | Exp Ratio | QIon | Exp Ratio |
|-----------------|-------|--------|-------|-----------|------|-----------|
| Trichloroethene | N.D.  | 7.03   | 130.0 | 101.5     | 97.0 | 64.1      |

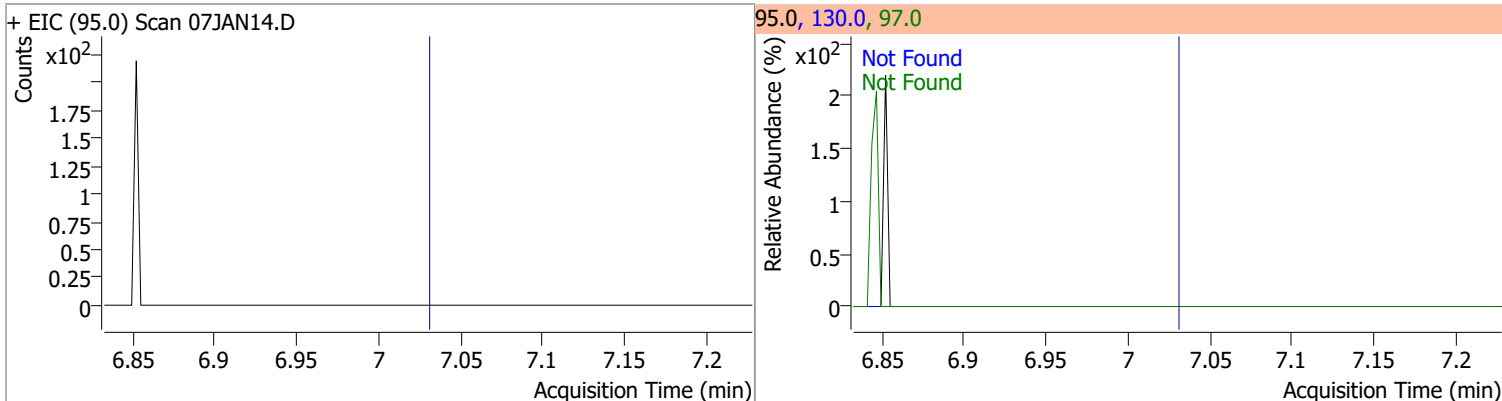


# Quantitation Results Report (QT Reviewed)

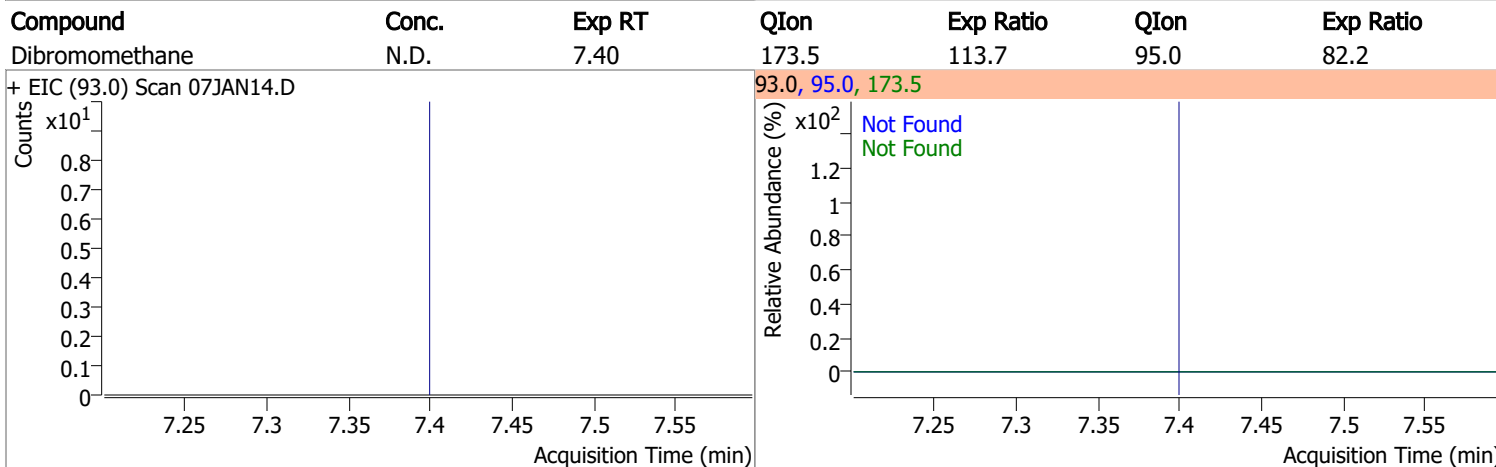


# Quantitation Results Report (QT Reviewed)


| Compound   | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 267.8901 | 8.32 | 0.00     | 856527 | 100.0 | 63.7   | 34.4  | 94.4  |
|            |          |      |          |        | 99.0  | 9.4    | 0.0   | 39.6  |

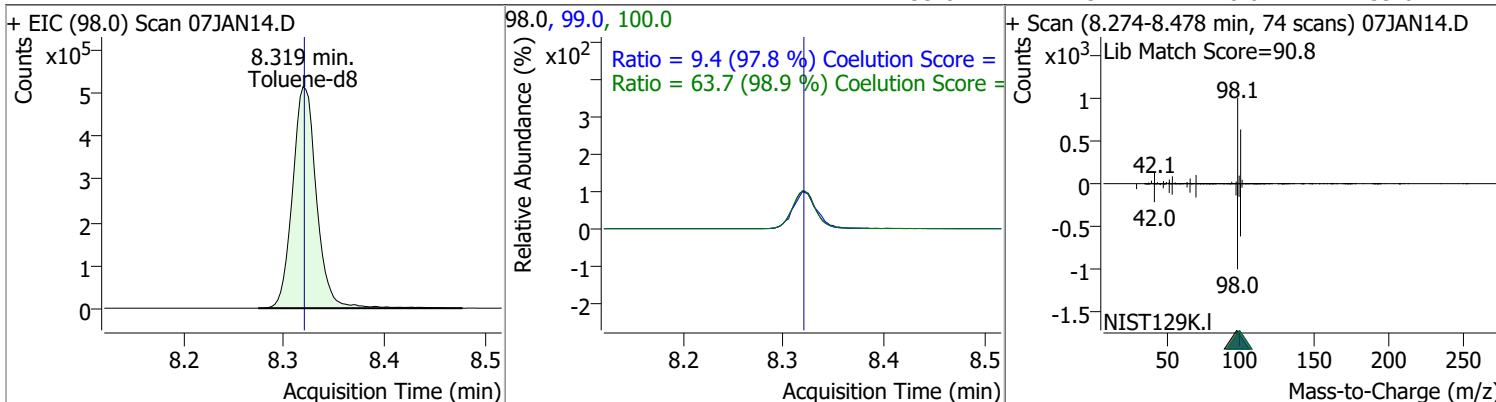


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|-------|----|----------|-------|------|--------|-------|-------|
| Toluene  | 0     | 0  | 0        | 0     | 91.0 | 145.8  | 205.8 |       |



| Compound                  | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,3-Dichloropropene | N.D.  | 8.64   | 39.0 | 53.4      | 77.0 | 32.4      |

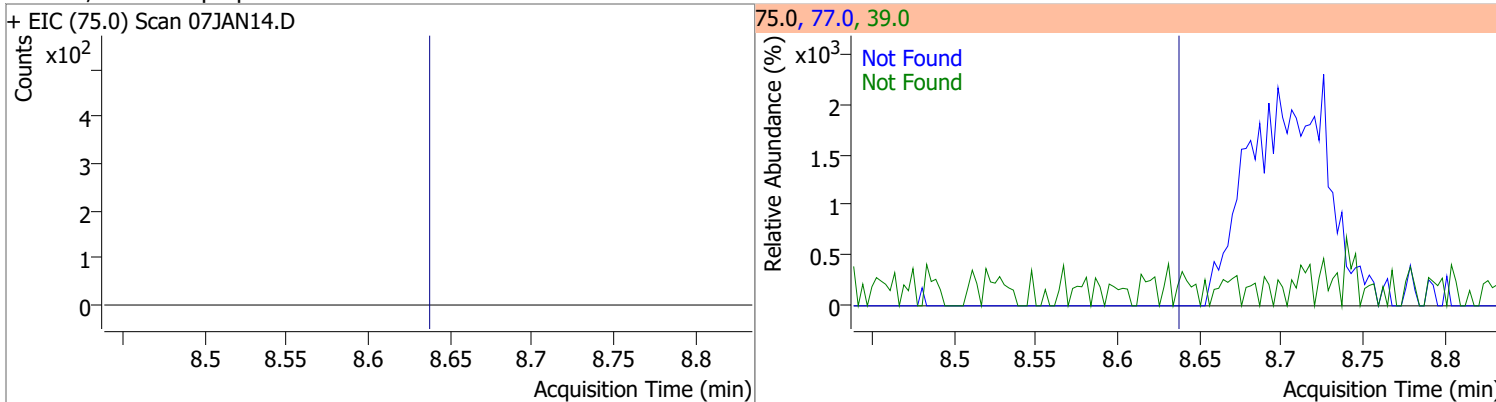


| Compound              | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------------|-------|--------|------|-----------|------|-----------|
| 1,1,2-Trichloroethane | N.D.  | 8.82   | 97.0 | 114.6     | 85.0 | 67.6      |

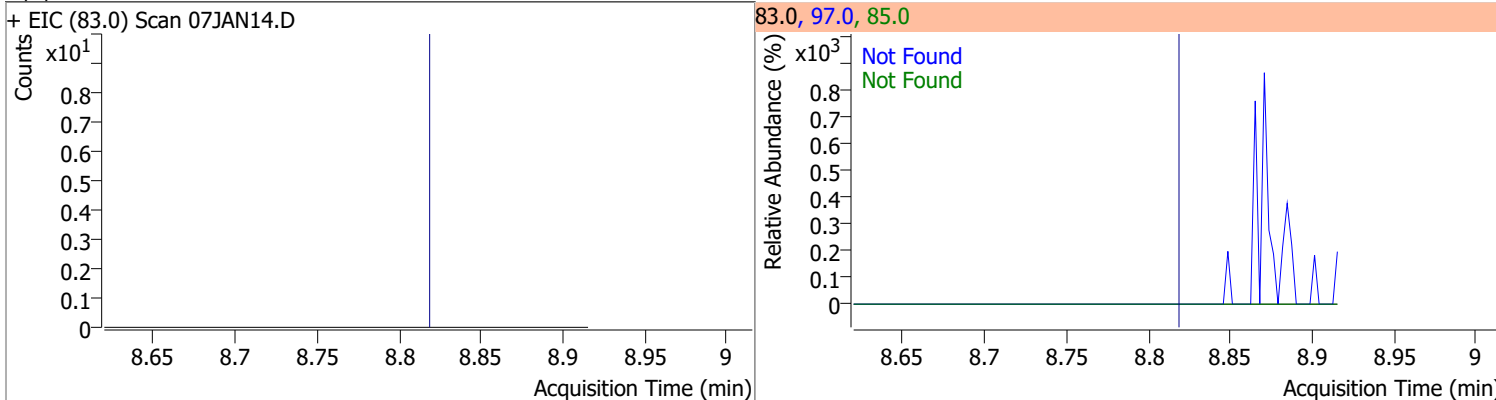


# Quantitation Results Report (QT Reviewed)


| Compound          | Conc. | Exp RT | QIon  | Exp Ratio | QIon  | Exp Ratio |
|-------------------|-------|--------|-------|-----------|-------|-----------|
| Tetrachloroethene | N.D.  | 8.94   | 165.8 | 128.6     | 129.0 | 91.5      |




| Compound            | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| 1,3-Dichloropropane | N.D.  | 8.98   | 78.0 | 32.9      |











| Compound             | Conc. | Exp RT | QIon  | Exp Ratio |
|----------------------|-------|--------|-------|-----------|
| Chlorodibromomethane | N.D.  | 9.21   | 127.0 | 78.0      |






| Compound          | Conc. | Exp RT | QIon  | Exp Ratio |
|-------------------|-------|--------|-------|-----------|
| 1,2-Dibromoethane | N.D.  | 9.31   | 109.0 | 94.5      |




# Quantitation Results Report (QT Reviewed)
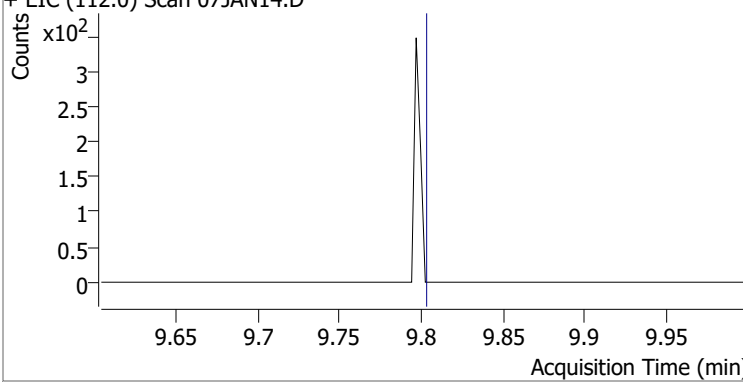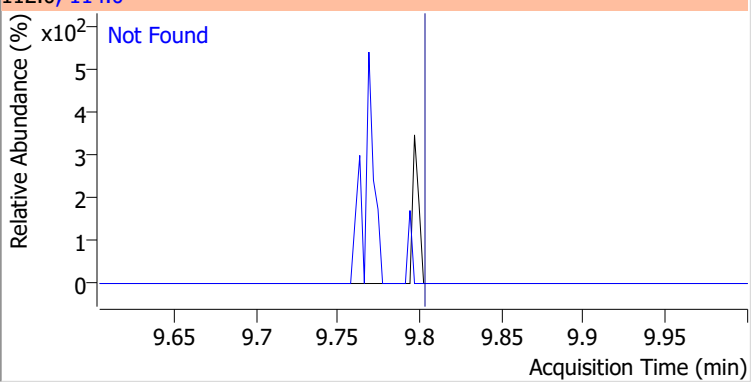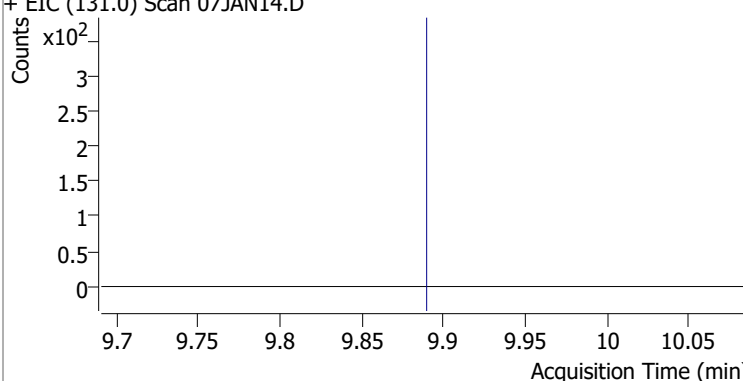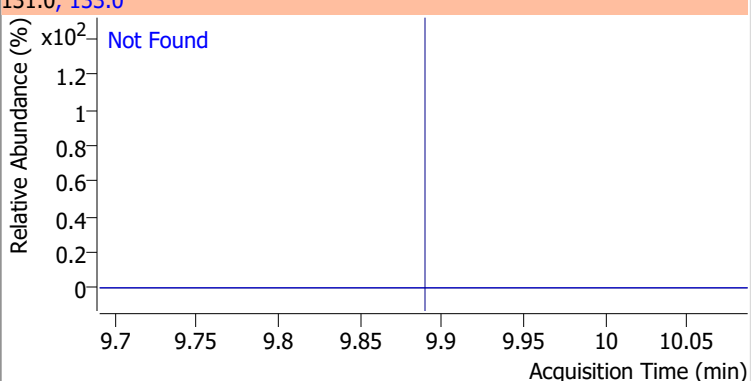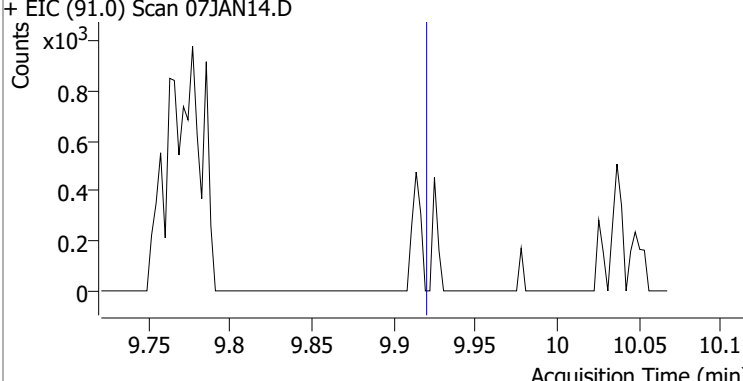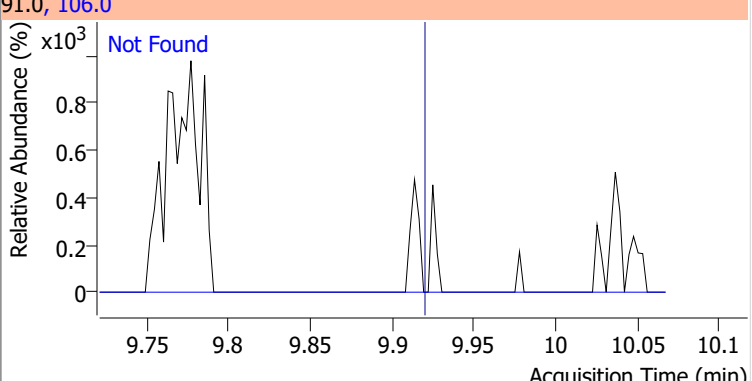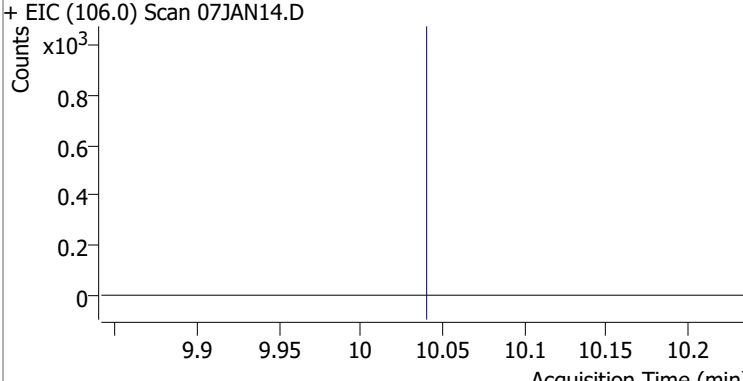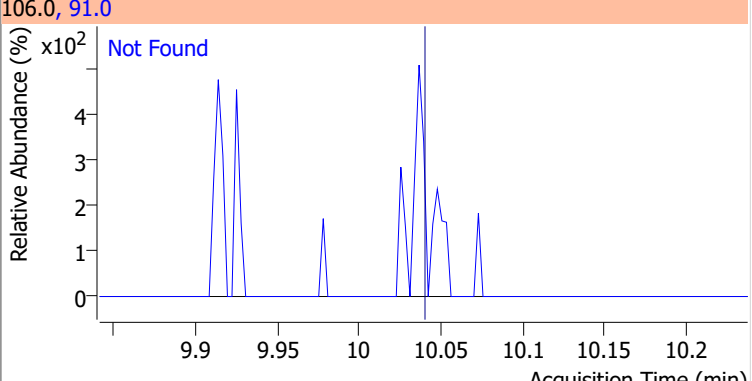
| Compound                                                                           | Conc. | Exp RT | QIon                                                                                 | Exp Ratio |
|------------------------------------------------------------------------------------|-------|--------|--------------------------------------------------------------------------------------|-----------|
| Chlorobenzene                                                                      | N.D.  | 9.80   | 114.0                                                                                | 32.1      |
| + EIC (112.0) Scan 07JAN14.D                                                       |       |        | 112.0, 114.0                                                                         |           |
|    |       |        |    |           |
| 1,1,1,2-Tetrachloroethane                                                          | N.D.  | 9.89   | 133.0                                                                                | 98.6      |
| + EIC (131.0) Scan 07JAN14.D                                                       |       |        | 131.0, 133.0                                                                         |           |
|   |       |        |   |           |
| Ethylbenzene                                                                       | N.D.  | 9.92   | 106.0                                                                                | 31.1      |
| + EIC (91.0) Scan 07JAN14.D                                                        |       |        | 91.0, 106.0                                                                          |           |
|  |       |        |  |           |
| m+p-Xylenes                                                                        | N.D.  | 10.04  | 91.0                                                                                 | 201.4     |
| + EIC (106.0) Scan 07JAN14.D                                                       |       |        | 106.0, 91.0                                                                          |           |
|  |       |        |  |           |









# Quantitation Results Report (QT Reviewed)

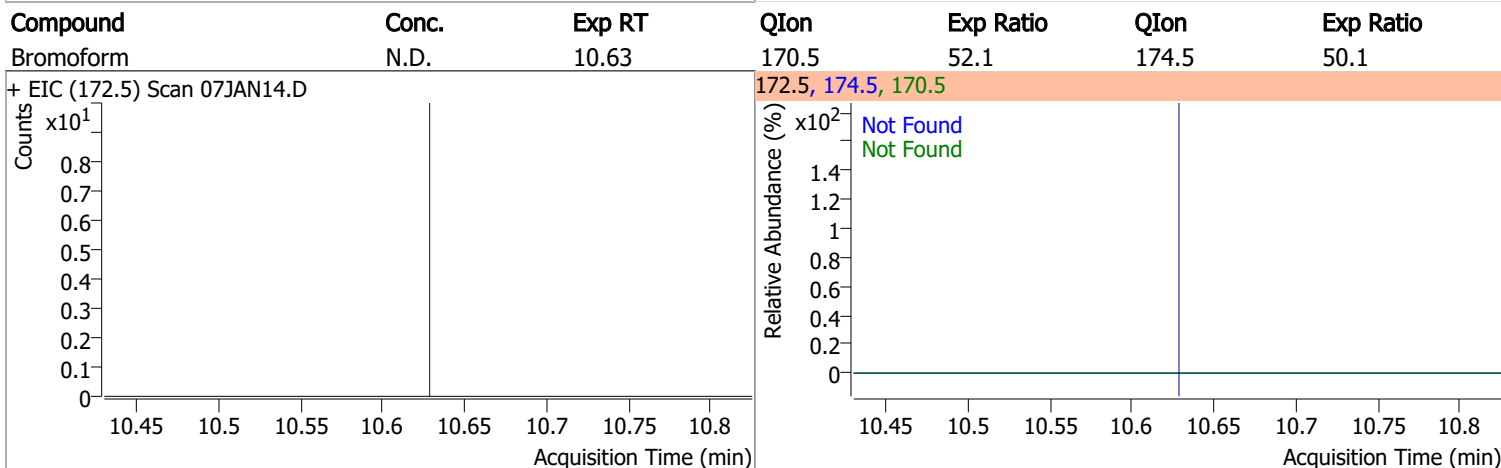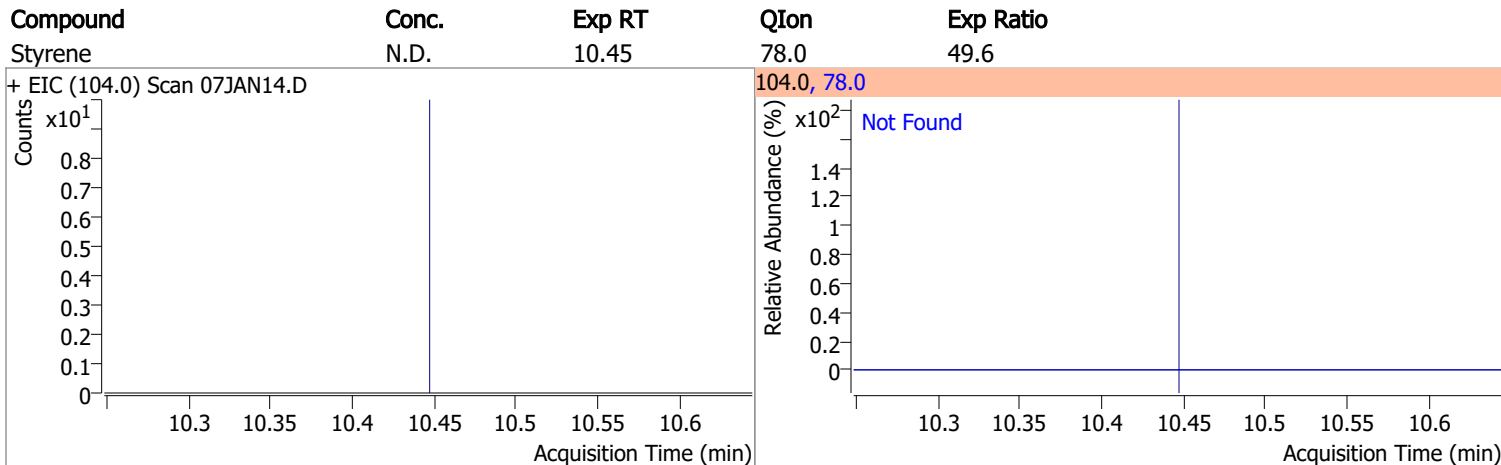









| Compound             | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 276.5273 | 10.95 | 0.00     | 255176 | 174.0 | 93.4   | 61.7  | 121.7 |
|                      |          |       |          |        | 176.0 | 89.1   | 60.6  | 120.6 |



# Quantitation Results Report (QT Reviewed)
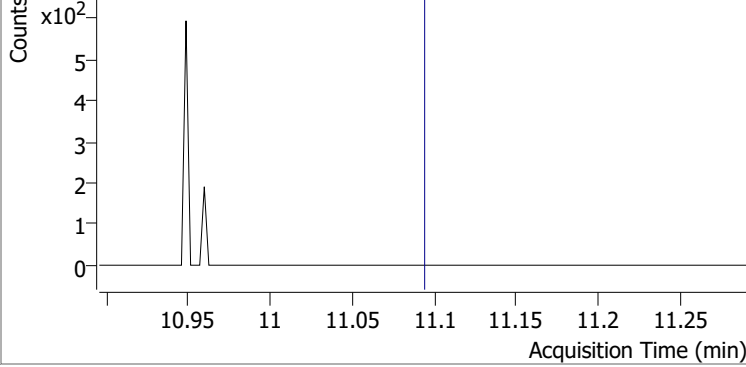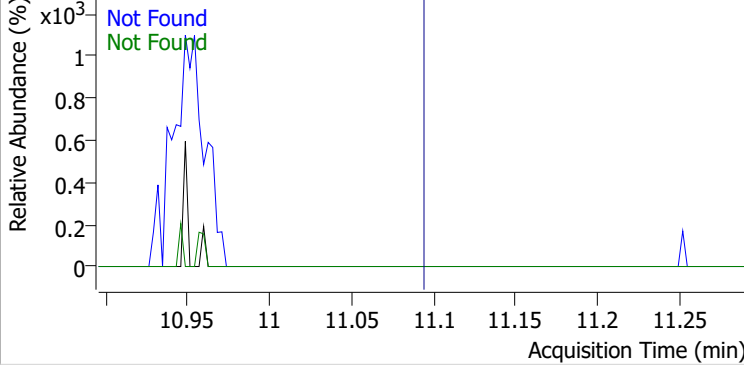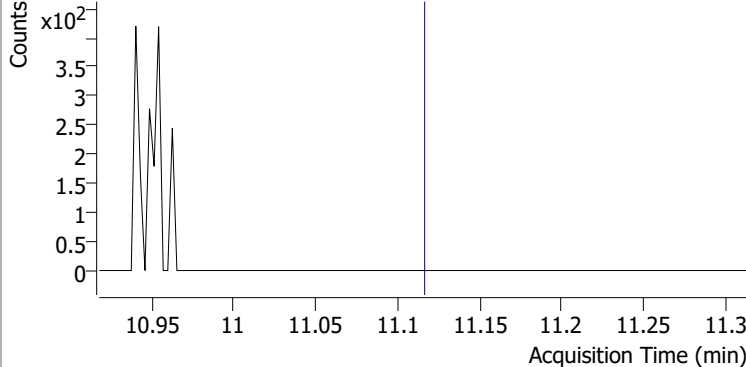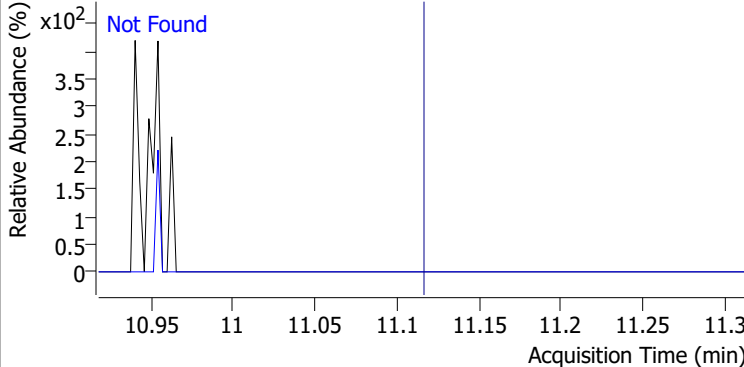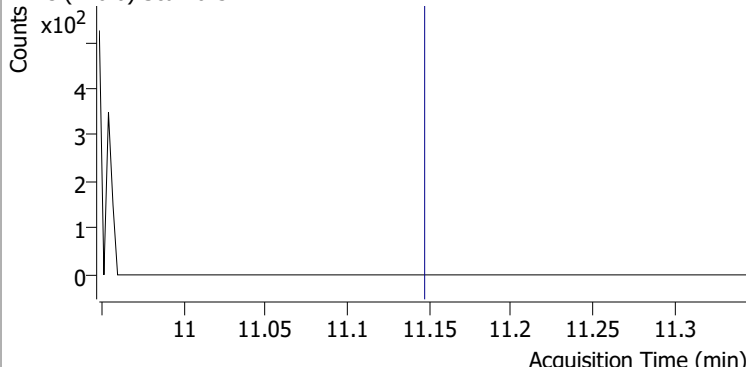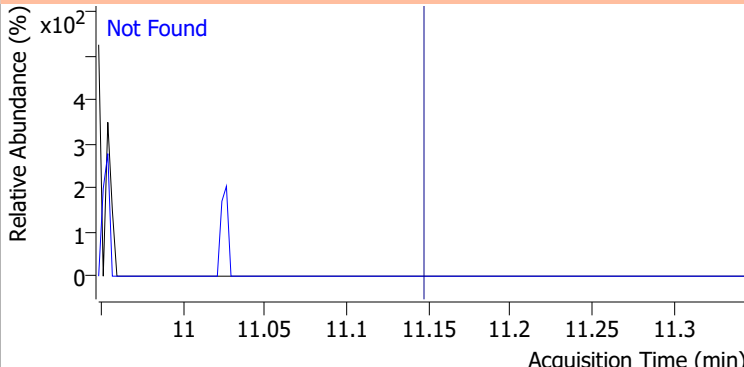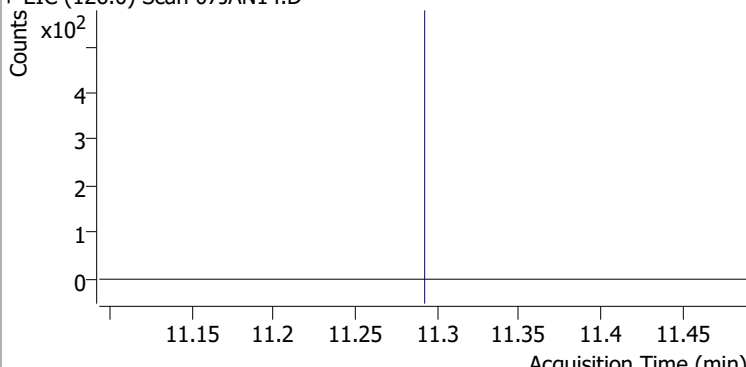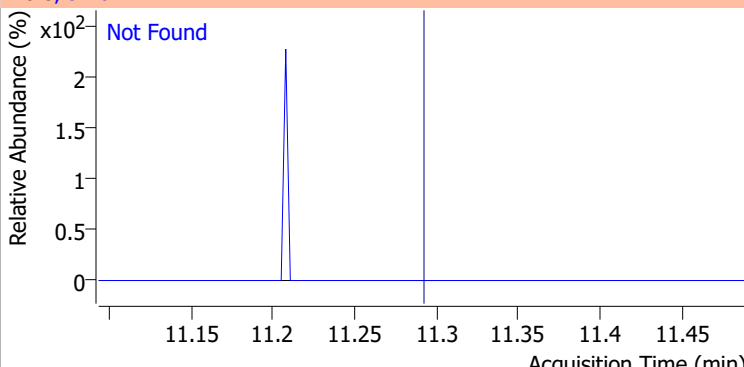
| Compound                                                                           | Conc. | Exp RT | QIon                                                                                 | Exp Ratio | QIon  | Exp Ratio |
|------------------------------------------------------------------------------------|-------|--------|--------------------------------------------------------------------------------------|-----------|-------|-----------|
| Bromobenzene                                                                       | N.D.  | 11.09  | 77.0                                                                                 | 145.7     | 158.0 | 96.5      |
| + EIC (156.0) Scan 07JAN14.D                                                       |       |        | 156.0, 77.0, 158.0                                                                   |           |       |           |
|    |       |        |    |           |       |           |
| 1,1,2-Tetrachloroethane                                                            | N.D.  | 11.12  | 85.0                                                                                 | 66.2      |       |           |
| + EIC (83.0) Scan 07JAN14.D                                                        |       |        | 83.0, 85.0                                                                           |           |       |           |
|   |       |        |   |           |       |           |
| 1,2,3-Trichloropropane                                                             | N.D.  | 11.15  | 112.0                                                                                | 63.5      |       |           |
| + EIC (110.0) Scan 07JAN14.D                                                       |       |        | 110.0, 112.0                                                                         |           |       |           |
|  |       |        |  |           |       |           |
| 2-Chlorotoluene                                                                    | N.D.  | 11.29  | 91.0                                                                                 | 282.3     |       |           |
| + EIC (126.0) Scan 07JAN14.D                                                       |       |        | 126.0, 91.0                                                                          |           |       |           |
|  |       |        |  |           |       |           |


# Quantitation Results Report (QT Reviewed)
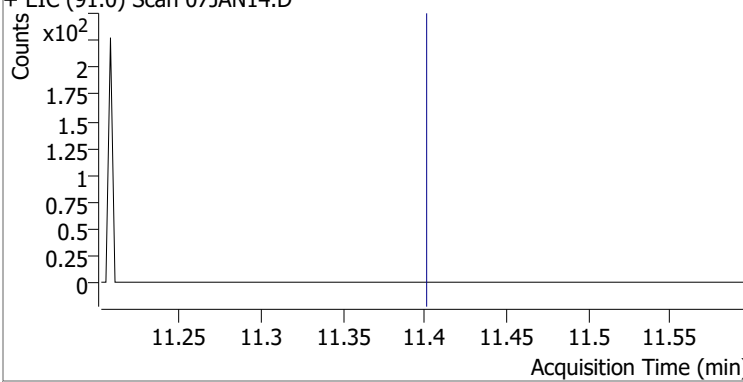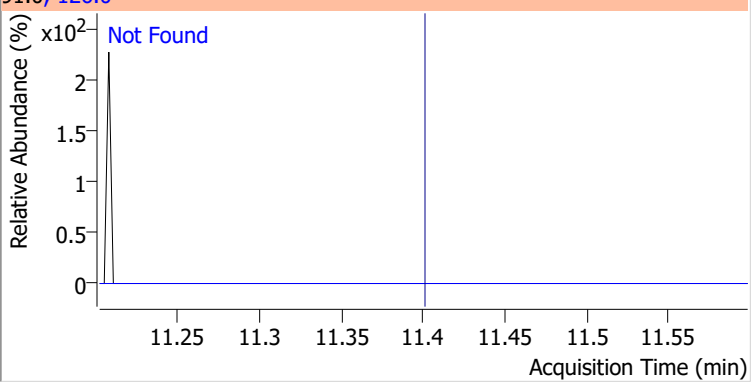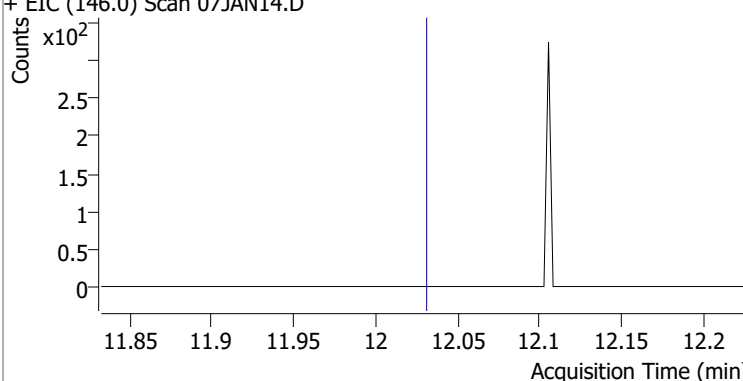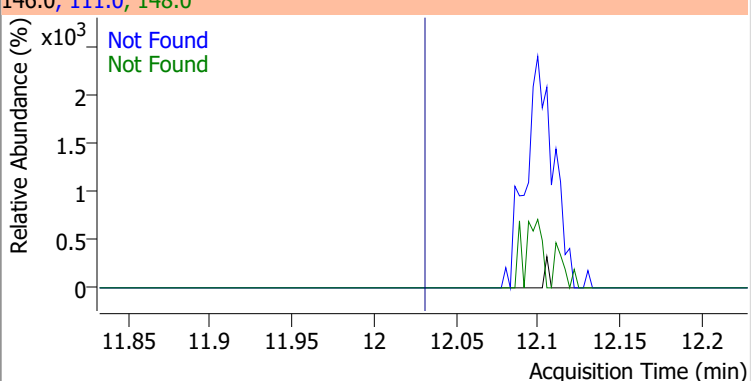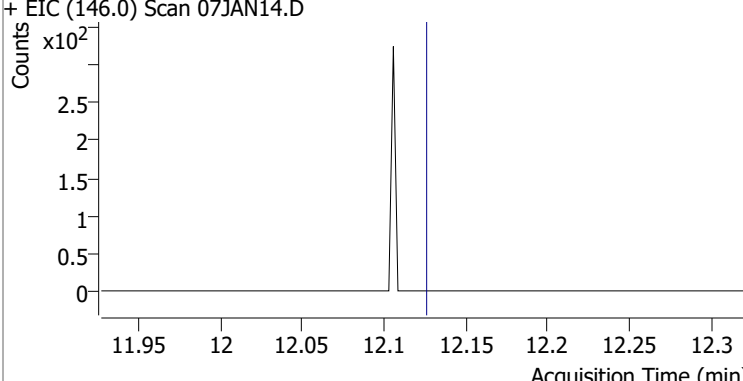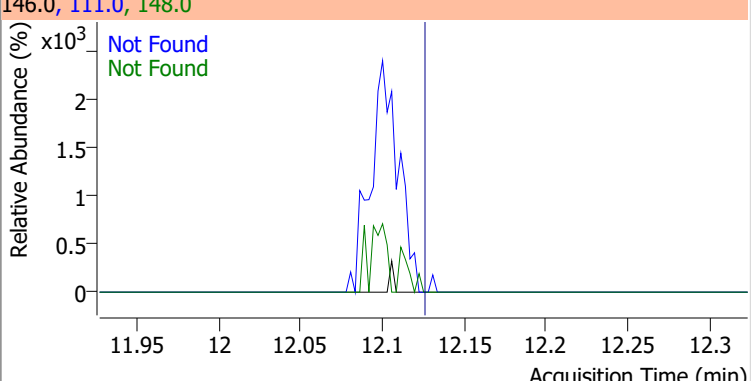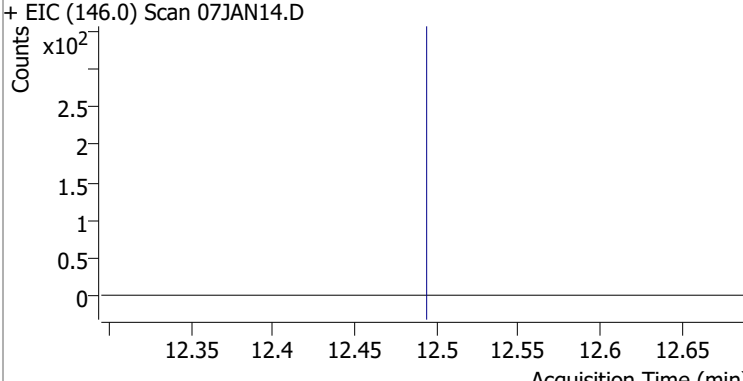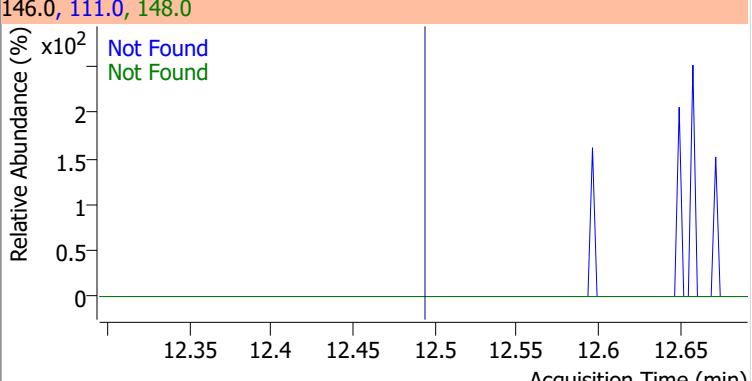
| Compound                                                                           | Conc. | Exp RT | QIon                                                                                 | Exp Ratio |      |           |
|------------------------------------------------------------------------------------|-------|--------|--------------------------------------------------------------------------------------|-----------|------|-----------|
| 4-Chlorotoluene                                                                    | N.D.  | 11.40  | 126.0                                                                                | 31.7      |      |           |
| + EIC (91.0) Scan 07JAN14.D                                                        |       |        | 91.0, 126.0                                                                          |           |      |           |
|    |       |        |    |           |      |           |
| 1,3-Dichlorobenzene                                                                | N.D.  | 12.03  | 148.0                                                                                | 63.6      | QIon | Exp Ratio |
| + EIC (146.0) Scan 07JAN14.D                                                       |       |        | 146.0, 111.0, 148.0                                                                  |           |      |           |
|   |       |        |   |           |      |           |
| 1,4-Dichlorobenzene                                                                | N.D.  | 12.13  | 148.0                                                                                | 63.1      | QIon | Exp Ratio |
| + EIC (146.0) Scan 07JAN14.D                                                       |       |        | 146.0, 111.0, 148.0                                                                  |           |      |           |
|  |       |        |  |           |      |           |
| 1,2-Dichlorobenzene                                                                | N.D.  | 12.49  | 148.0                                                                                | 63.9      | QIon | Exp Ratio |
| + EIC (146.0) Scan 07JAN14.D                                                       |       |        | 146.0, 111.0, 148.0                                                                  |           |      |           |
|  |       |        |  |           |      |           |



# Quantitation Results Report (QT Reviewed)

|                |                                     |                   |                       |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File      | 07JAN15.D                           | Operator          | MSC                   |
| Acq. Method    | 5975CACQF.M                         | Acq. Date-Time    | 1/7/2022 4:03:14 PM   |
| Sample Name    | B22010262-001F                      | Instrument        | VOA5975C              |
| Vial           | 15                                  | Multiplier        | 1.00                  |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m  | Comment           |                       |
| Tune File      | BFB_Atune3.u                        | Tune Date         | 10/11/2021 4:02:00 PM |
| Batch Name     | VG010722_8260B.batch.bin            | Last Calib Update | 3/2/2022 10:41:44 AM  |
| Ref Library    | \\MASSHUNTER\Org\Library\NIST129K.I |                   |                       |

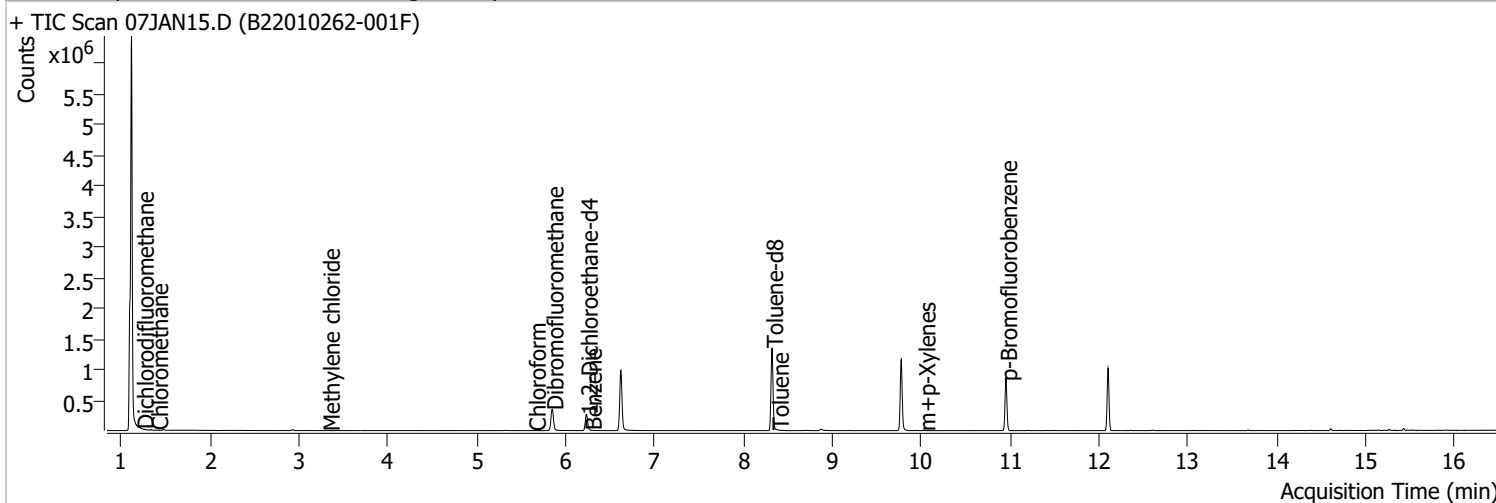





| Compound                           | RT                   | QIon  | Resp.  | Conc.              | Units | Dev(Min) |    |
|------------------------------------|----------------------|-------|--------|--------------------|-------|----------|----|
| <b>Internal Standards</b>          |                      |       |        |                    |       |          |    |
| M Fluorobenzene                    | 6.620                | 96.0  | 829021 | 250.0000           | ng    | -0.003   |    |
| M Chlorobenzene-d5                 | 9.774                | 82.0  | 317136 | 250.0000           | ng    | 0.003    |    |
| M 1,4-Dichlorobenzene-d4           | 12.100               | 152.0 | 243125 | 250.0000           | ng    | 0.000    |    |
| <b>System Monitoring Compounds</b> |                      |       |        |                    |       |          |    |
| S Dibromofluoromethane             | 5.851                | 113.0 | 213658 | 273.5621           | ng    | 0.005    |    |
| Spiked Amount: 250.000             | Range: 80.0 - 119.0% |       |        | Recovery = 109.42% |       |          |    |
| S 1,2-Dichloroethane-d4            | 6.236                | 67.0  | 96525  | 286.1313           | ng    | 0.003    |    |
| Spiked Amount: 250.000             | Range: 81.0 - 118.0% |       |        | Recovery = 114.45% |       |          |    |
| S Toluene-d8                       | 8.321                | 98.0  | 826770 | 270.5325           | ng    | 0.003    |    |
| Spiked Amount: 250.000             | Range: 89.0 - 112.0% |       |        | Recovery = 108.21% |       |          |    |
| S p-Bromofluorobenzene             | 10.954               | 95.0  | 240345 | 269.8409           | ng    | 0.000    |    |
| Spiked Amount: 250.000             | Range: 85.0 - 114.0% |       |        | Recovery = 107.94% |       |          |    |
| <b>Target Compounds</b>            |                      |       |        |                    |       |          |    |
| T Dichlorodifluoromethane          | 1.241                | 85.0  | 1185   | 1.0904             | ng    | m        | 95 |
| T Chloromethane                    | 1.406                | 50.0  | 626    | 0.4748             | ng    | m        | 60 |
| T Vinyl chloride                   | 0.000                |       | 0      | N.D.               |       |          |    |
| T Bromomethane                     | 0.000                |       | 0      | N.D.               |       |          |    |
| T Chloroethane                     | 0.000                |       | 0      | N.D.               |       |          |    |
| T Trichlorofluoromethane           | 0.000                |       | 0      | N.D.               |       |          |    |
| T 1,1-Dichloroethene               | 0.000                |       | 0      | N.D.               |       |          |    |
| T Methylene chloride               | 3.335                | 49.0  | 648    | 0.5261             | ng    | m        | 98 |
| T trans-1,2-Dichloroethene         | 0.000                |       | 0      | N.D.               |       |          |    |
| T Methyl tert-butyl ether (MTBE)   | 0.000                |       | 0      | N.D.               |       |          |    |
| T 1,1-Dichloroethane               | 0.000                |       | 0      | N.D.               |       |          |    |
| T 2,2-Dichloropropane              | 0.000                |       | 0      | N.D.               |       |          |    |
| T cis-1,2-Dichloroethene           | 0.000                |       | 0      | N.D.               |       |          |    |
| T Methyl ethyl ketone              | 0.000                |       | 0      | N.D.               |       |          |    |
| T Bromochloromethane               | 0.000                |       | 0      | N.D.               |       |          |    |
| T Chloroform                       | 5.653                | 83.0  | 600    | 0.3801             | ng    | #m       | 35 |

# Quantitation Results Report (QT Reviewed)

| Compound                    | RT     | QIon  | Resp. | Conc.  | Units |    | Dev(Min) |
|-----------------------------|--------|-------|-------|--------|-------|----|----------|
| T 1,1,1-Trichloroethane     | 0.000  |       | 0     | N.D.   |       |    |          |
| T Carbon tetrachloride      | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,1-Dichloropropene       | 0.000  |       | 0     | N.D.   |       |    |          |
| T Benzene                   | 6.283  | 78.0  | 748   | 0.2266 | ng    | m  | 81       |
| T 1,2-Dichloroethane        | 0.000  |       | 0     | N.D.   |       |    |          |
| T Trichloroethene           | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,2-Dichloropropane       | 0.000  |       | 0     | N.D.   |       |    |          |
| T Dibromomethane            | 0.000  |       | 0     | N.D.   |       |    |          |
| T Bromodichloromethane      | 0.000  |       | 0     | N.D.   |       |    |          |
| T cis-1,3-Dichloropropene   | 0.000  |       | 0     | N.D.   |       |    |          |
| T Toluene                   | 8.386  | 92.0  | 723   | 0.3502 | ng    | m  | 100      |
| T trans-1,3-Dichloropropene | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,1,2-Trichloroethane     | 0.000  |       | 0     | N.D.   |       |    |          |
| T Tetrachloroethene         | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,3-Dichloropropane       | 0.000  |       | 0     | N.D.   |       |    |          |
| T Chlorodibromomethane      | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,2-Dibromoethane         | 0.000  |       | 0     | N.D.   |       |    |          |
| T Chlorobenzene             | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,1,1,2-Tetrachloroethane | 0.000  |       | 0     | N.D.   |       |    |          |
| T Ethylbenzene              | 0.000  |       | 0     | N.D.   |       |    |          |
| T m+p-Xylenes               | 10.036 | 106.0 | 505   | 0.3315 | ng    | m  | 87       |
| T o-Xylene                  | 10.427 | 106.0 | 0     |        | ng    | md | 1        |
| T Styrene                   | 0.000  |       | 0     | N.D.   |       |    |          |
| T Bromoform                 | 0.000  |       | 0     | N.D.   |       |    |          |
| T Bromobenzene              | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,1,2,2-Tetrachloroethane | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,2,3-Trichloropropane    | 0.000  |       | 0     | N.D.   |       |    |          |
| T 2-Chlorotoluene           | 0.000  |       | 0     | N.D.   |       |    |          |
| T 4-Chlorotoluene           | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,3-Dichlorobenzene       | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,4-Dichlorobenzene       | 0.000  |       | 0     | N.D.   |       |    |          |
| T 1,2-Dichlorobenzene       | 0.000  |       | 0     | N.D.   |       |    |          |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (\*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

# Quantitation Results Report (QT Reviewed)

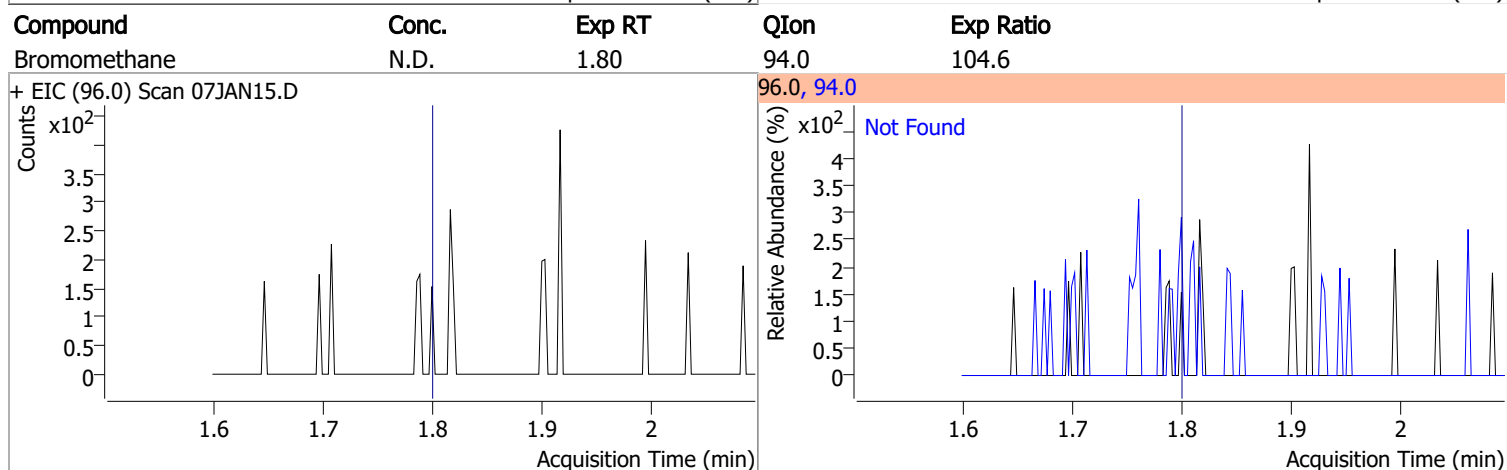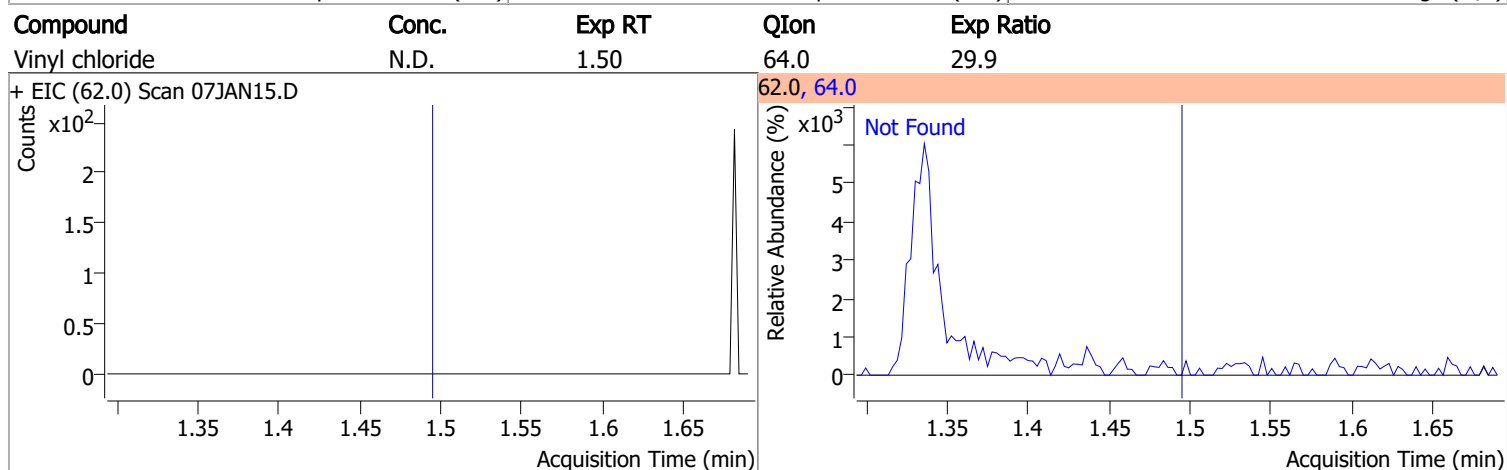


# Quantitation Results Report (QT Reviewed)


| Compound     | Conc. | Exp RT | QIon | Exp Ratio |
|--------------|-------|--------|------|-----------|
| Chloroethane | N.D.  | 1.89   | 66.0 | 30.1      |

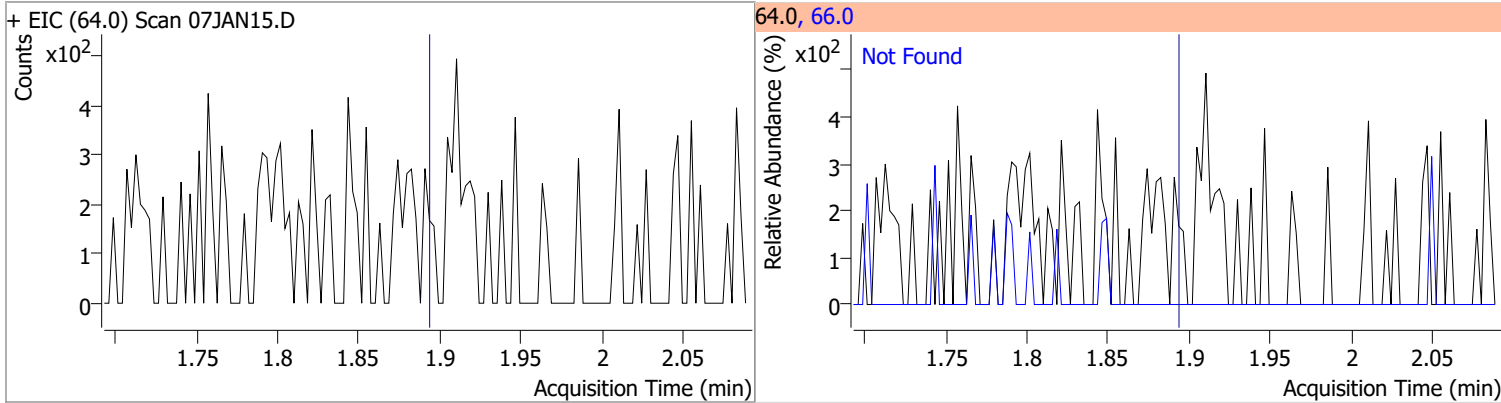


| Compound               | Conc. | Exp RT | QIon  | Exp Ratio |
|------------------------|-------|--------|-------|-----------|
| Trichlorofluoromethane | N.D.  | 2.14   | 103.0 | 64.2      |

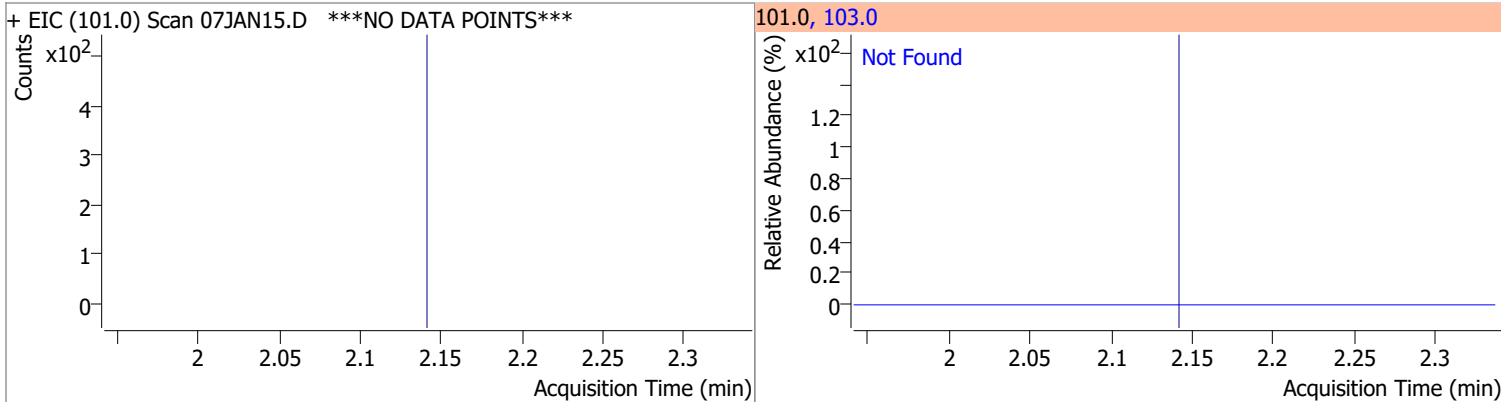

| Compound           | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethene | N.D.  | 2.70   | 61.0 | 180.3     | 63.0 | 56.7      |

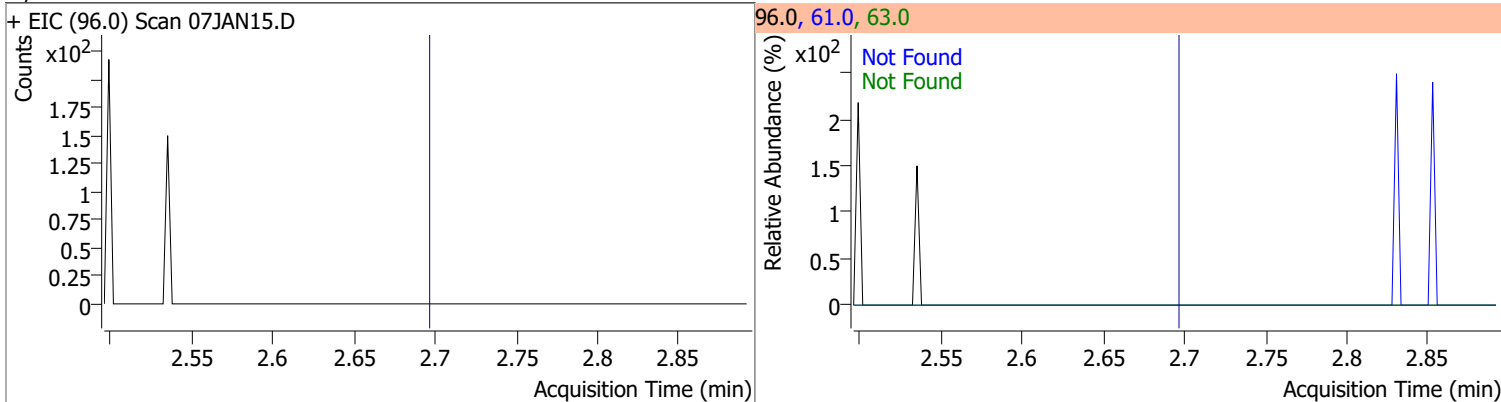


| Compound           | Conc.  | RT   | Dev(Min) | Resp.   | QIon | QRatio | Lower | Upper |
|--------------------|--------|------|----------|---------|------|--------|-------|-------|
| Methylene chloride | 0.5261 | 3.34 | 0.00     | 648 (m) | 84.0 | 69.5   | 36.9  | 96.9  |
|                    |        |      |          |         | 86.0 | 43.9   | 14.3  | 74.3  |




# Quantitation Results Report (QT Reviewed)


| Compound                 | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,2-Dichloroethene | N.D.  | 3.72   | 61.0 | 153.9     | 98.0 | 65.7      |




| Compound                       | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------------------|-------|--------|------|-----------|
| Methyl tert-butyl ether (MTBE) | N.D.  | 3.75   | 57.0 | 24.6      |



| Compound           | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,1-Dichloroethane | N.D.  | 4.38   | 65.0 | 32.1      | 83.0 | 13.7      |




| Compound            | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|------|-----------|
| 2,2-Dichloropropane | N.D.  | 5.20   | 41.0 | 66.5      | 97.0 | 23.2      |




# Quantitation Results Report (QT Reviewed)


| Compound               | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|------------------------|-------|--------|------|-----------|------|-----------|
| cis-1,2-Dichloroethene | N.D.  | 5.22   | 61.0 | 167.2     | 98.0 | 67.3      |




| Compound            | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| Methyl ethyl ketone | N.D.  | 5.28   | 72.0 | 21.3      |







| Compound           | Conc. | Exp RT | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|
| Bromochloromethane | N.D.  | 5.52   | 49.0 | 182.9     |



| Compound   | Conc.  | RT   | Dev(Min) | Resp.   | QIon | QRatio | Lower | Upper |
|------------|--------|------|----------|---------|------|--------|-------|-------|
| Chloroform | 0.3801 | 5.65 | 0.00     | 600 (m) | 85.0 | 14.6   | 36.0  | 96.0  |




# Quantitation Results Report (QT Reviewed)

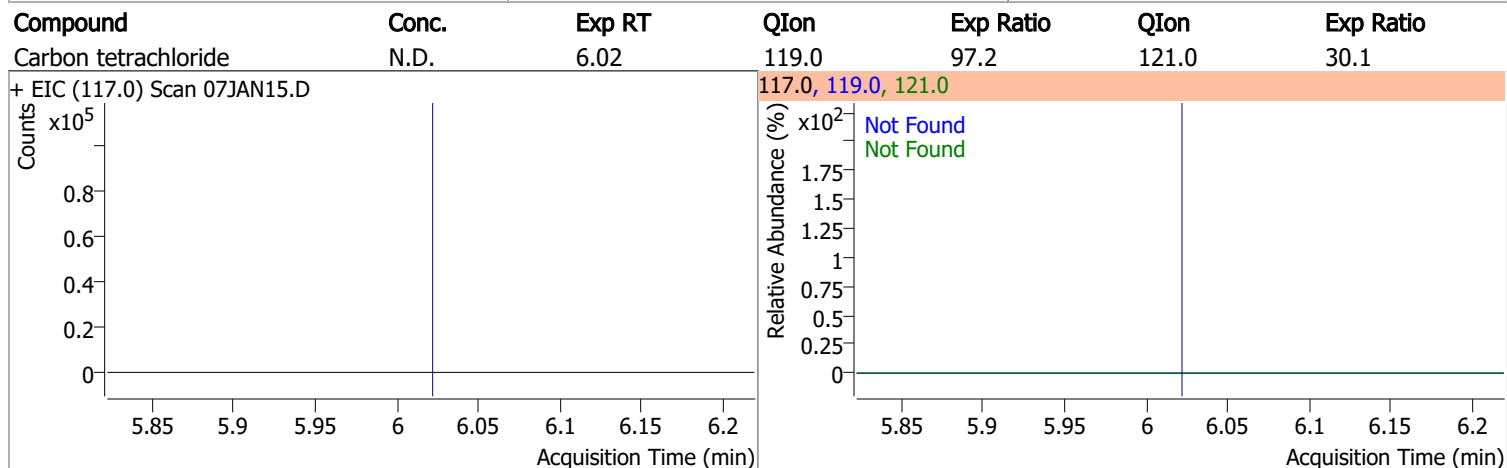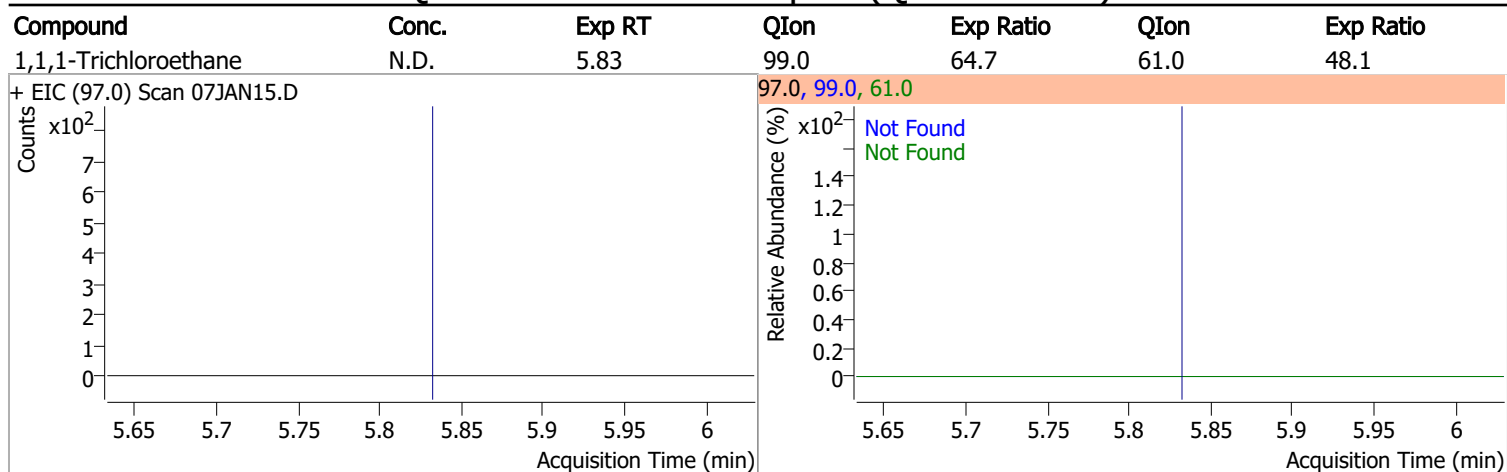


# Quantitation Results Report (QT Reviewed)


| Compound              | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 286.1313 | 6.24 | 0.00     | 96525 | 65.0 | 197.8  | 166.5 | 226.5 |




| Compound | Conc.  | RT   | Dev(Min) | Resp.   | QIon | QRatio | Lower | Upper |
|----------|--------|------|----------|---------|------|--------|-------|-------|
| Benzene  | 0.2266 | 6.28 | 0.01     | 748 (m) | 77.0 | 14.4   | 0.0   | 53.5  |



| Compound           | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|--------------------|-------|--------|------|-----------|------|-----------|
| 1,2-Dichloroethane | N.D.  | 6.32   | 64.0 | 29.9      | 98.0 | 7.6       |







| Compound        | Conc. | Exp RT | QIon  | Exp Ratio | QIon | Exp Ratio |
|-----------------|-------|--------|-------|-----------|------|-----------|
| Trichloroethene | N.D.  | 7.03   | 130.0 | 101.5     | 97.0 | 64.1      |






# Quantitation Results Report (QT Reviewed)

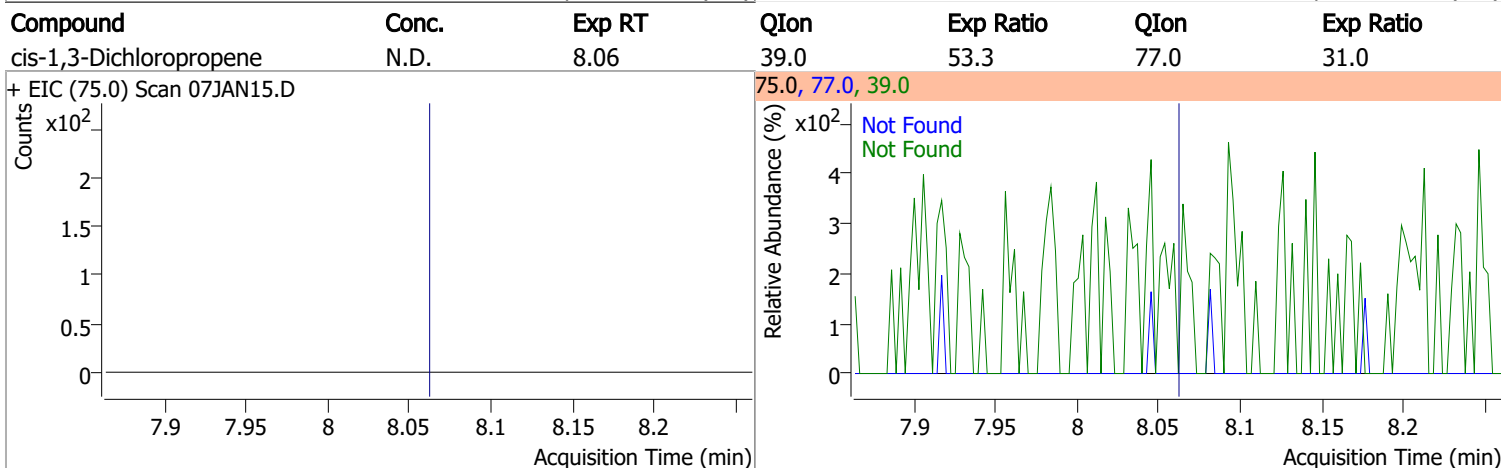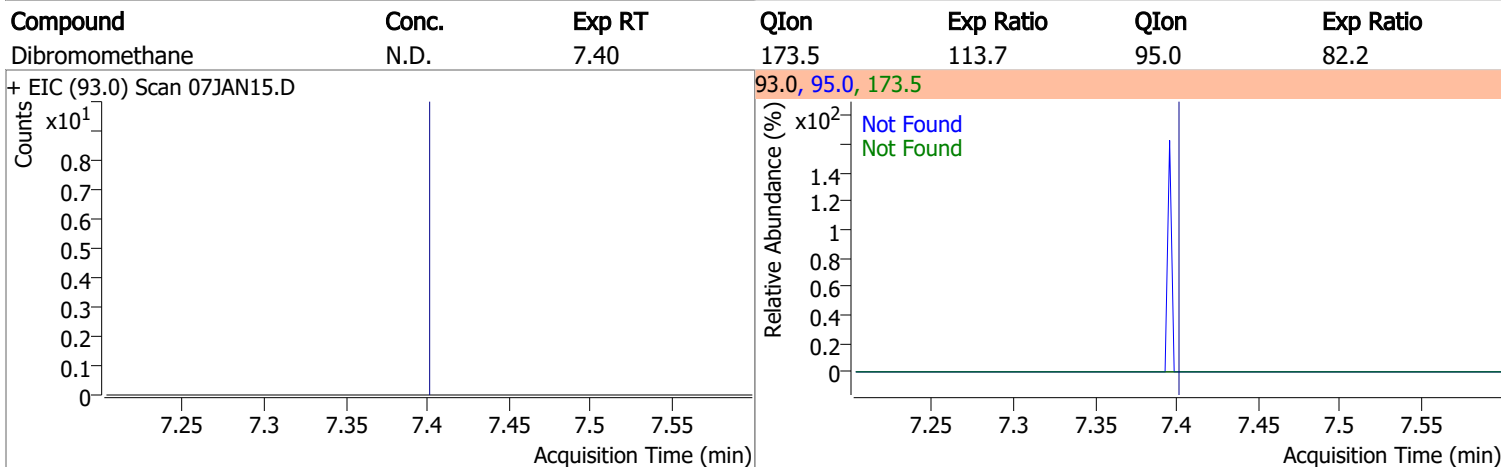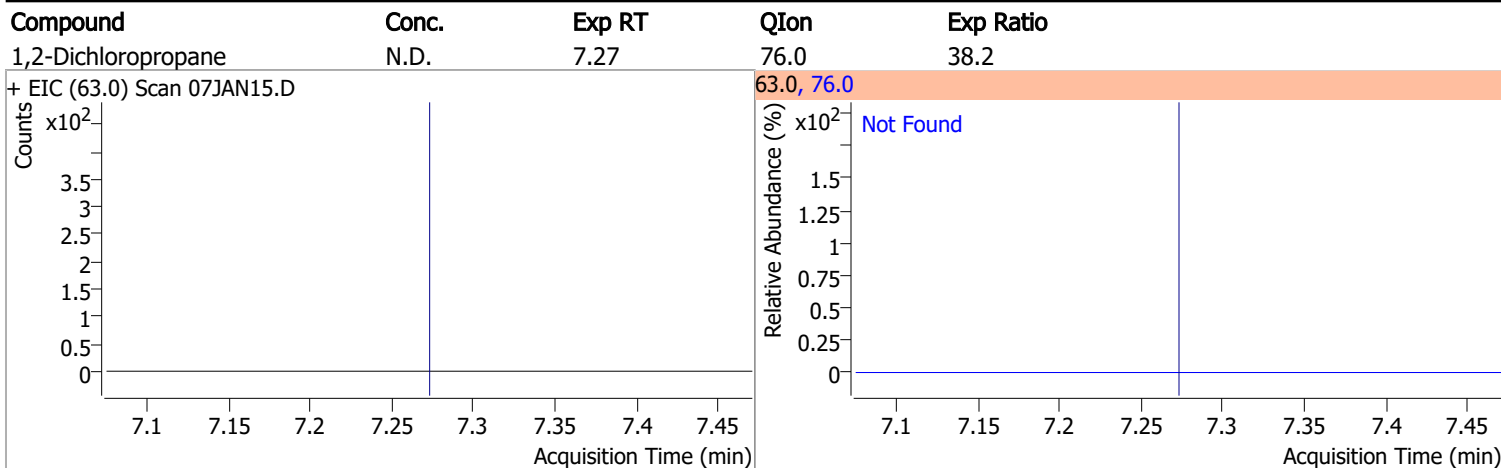


# Quantitation Results Report (QT Reviewed)


| Compound   | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 270.5325 | 8.32 | 0.00     | 826770 | 100.0 | 64.2   | 34.4  | 94.4  |
|            |          |      |          |        | 99.0  | 9.7    | 0.0   | 39.6  |




| Compound | Conc.  | RT   | Dev(Min) | Resp.   | QIon | QRatio | Lower | Upper |
|----------|--------|------|----------|---------|------|--------|-------|-------|
| Toluene  | 0.3502 | 8.39 | 0.00     | 723 (m) | 91.0 | 175.8  | 145.8 | 205.8 |



| Compound                  | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|---------------------------|-------|--------|------|-----------|------|-----------|
| trans-1,3-Dichloropropene | N.D.  | 8.64   | 39.0 | 53.4      | 77.0 | 32.4      |




| Compound              | Conc. | Exp RT | QIon | Exp Ratio | QIon | Exp Ratio |
|-----------------------|-------|--------|------|-----------|------|-----------|
| 1,1,2-Trichloroethane | N.D.  | 8.82   | 97.0 | 114.6     | 85.0 | 67.6      |




# Quantitation Results Report (QT Reviewed)


| Compound          | Conc. | Exp RT | QIon  | Exp Ratio | QIon  | Exp Ratio |
|-------------------|-------|--------|-------|-----------|-------|-----------|
| Tetrachloroethene | N.D.  | 8.94   | 165.8 | 128.6     | 129.0 | 91.5      |

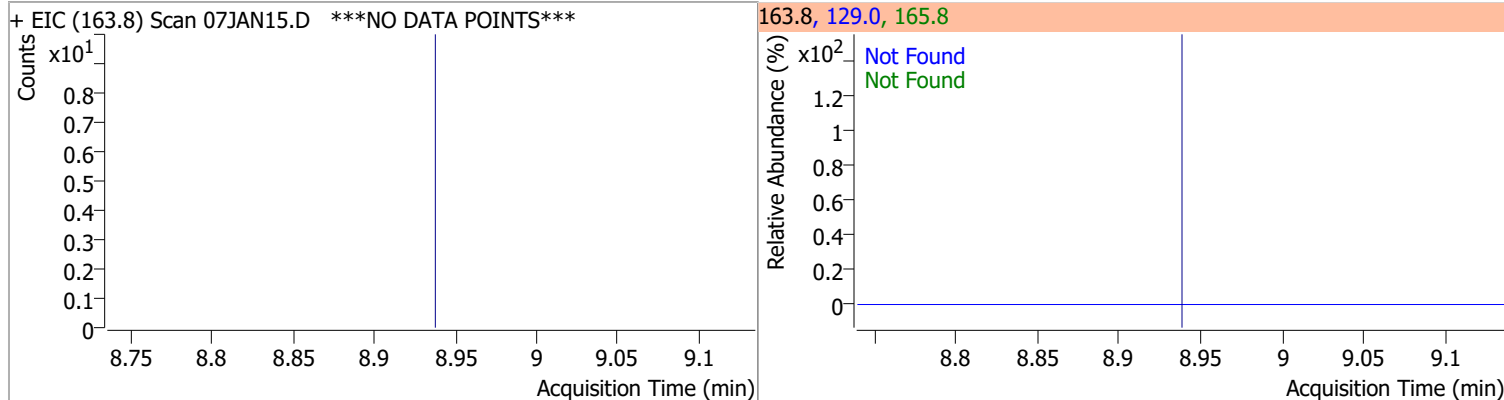


| Compound            | Conc. | Exp RT | QIon | Exp Ratio |
|---------------------|-------|--------|------|-----------|
| 1,3-Dichloropropane | N.D.  | 8.98   | 78.0 | 32.9      |

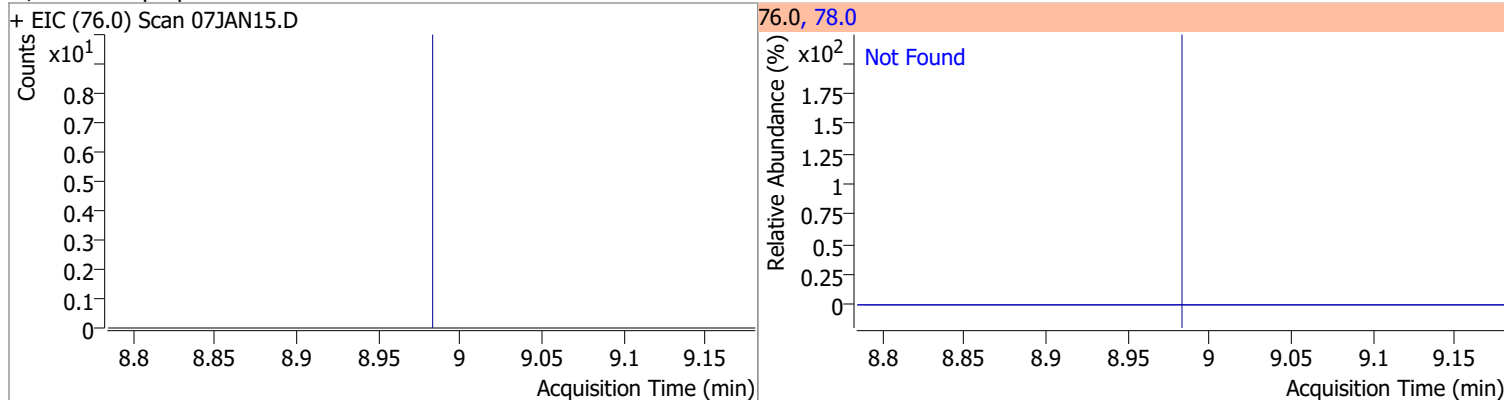







| Compound             | Conc. | Exp RT | QIon  | Exp Ratio |
|----------------------|-------|--------|-------|-----------|
| Chlorodibromomethane | N.D.  | 9.21   | 127.0 | 78.0      |



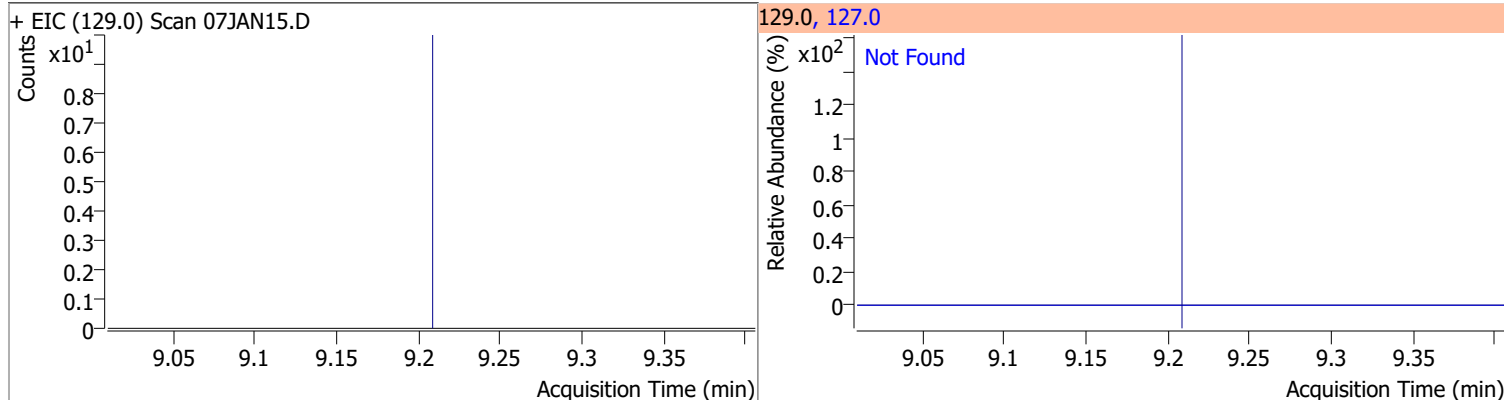


| Compound          | Conc. | Exp RT | QIon  | Exp Ratio |
|-------------------|-------|--------|-------|-----------|
| 1,2-Dibromoethane | N.D.  | 9.31   | 109.0 | 94.5      |

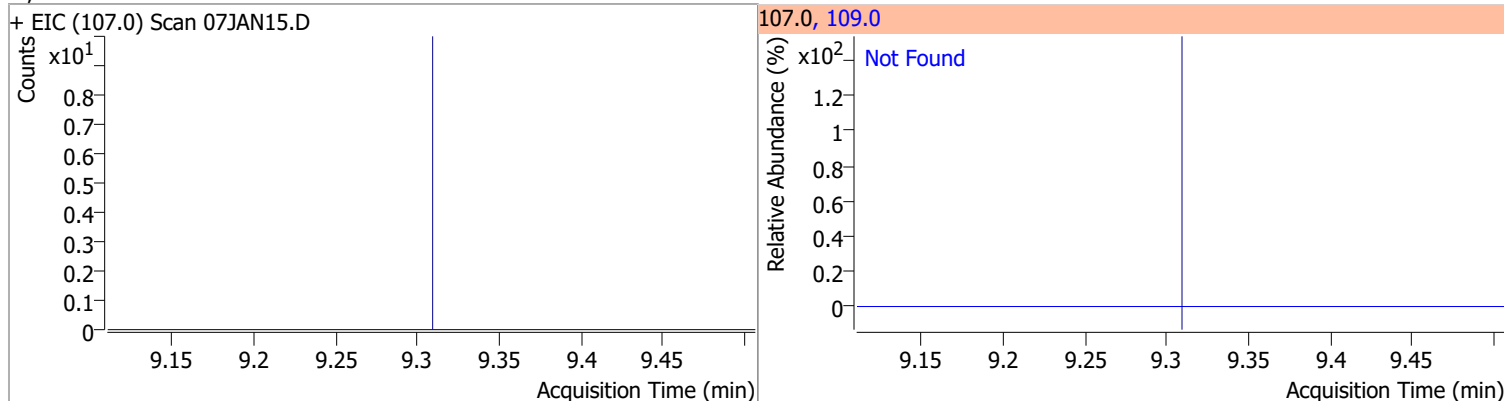


# Quantitation Results Report (QT Reviewed)
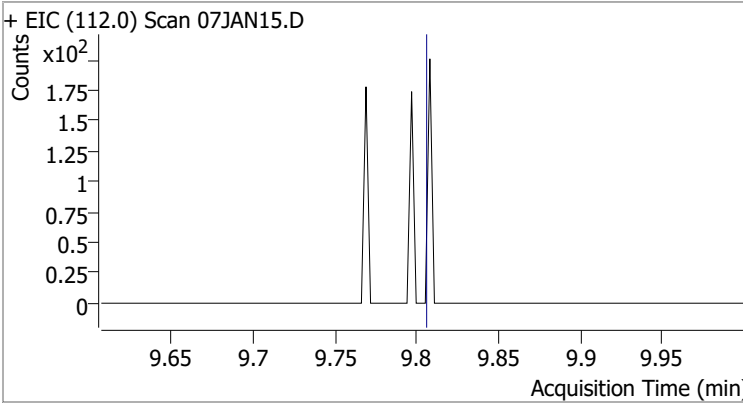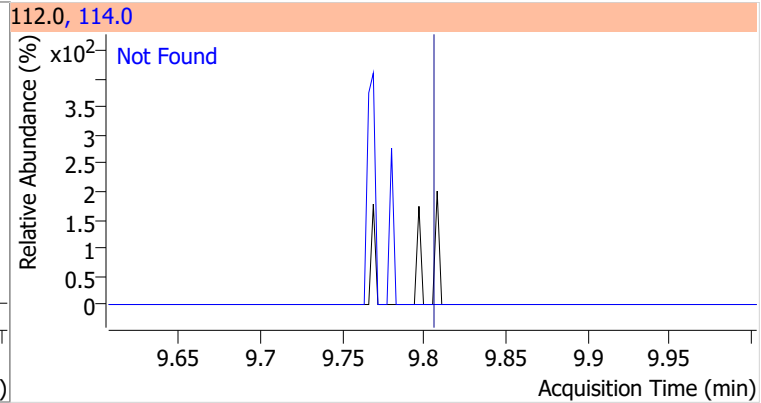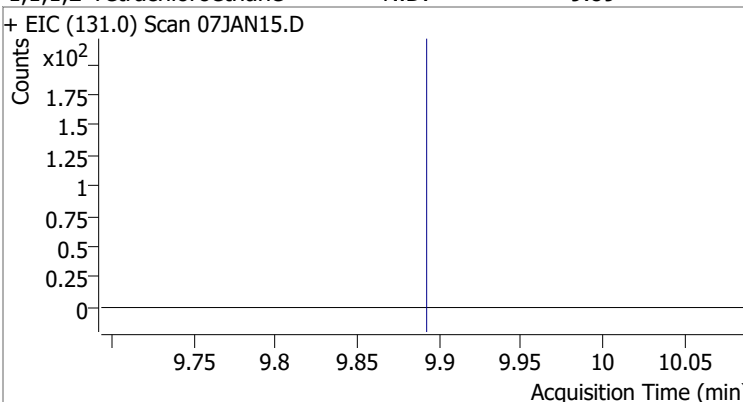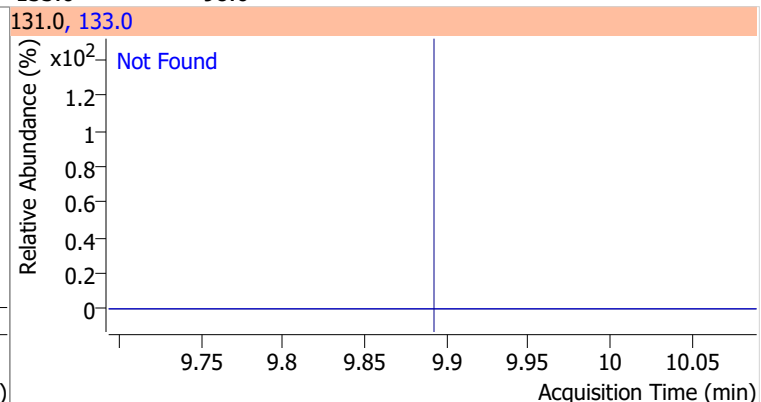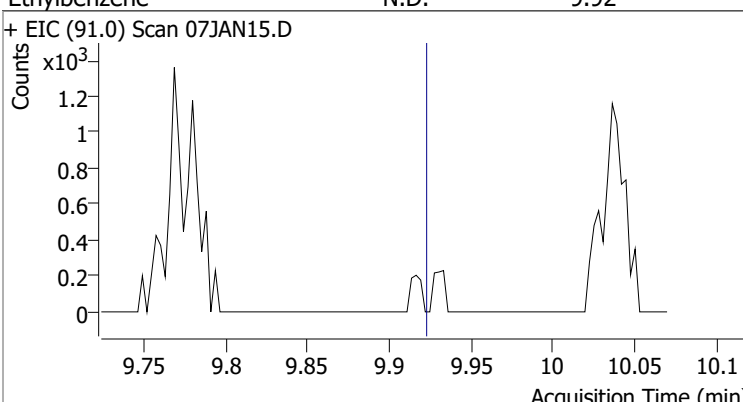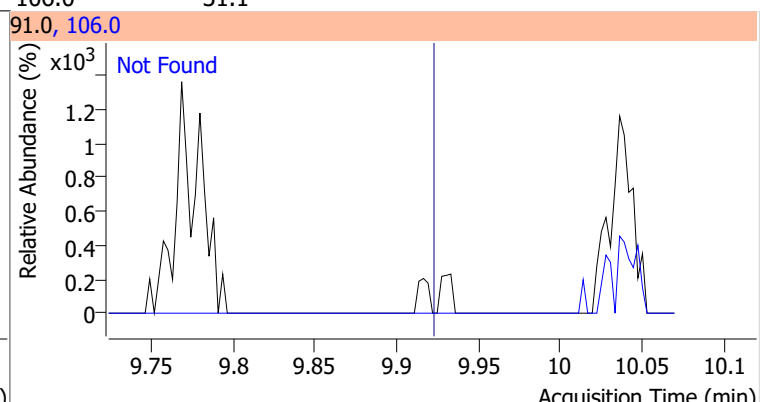
| Compound                                                                           | Conc. | Exp RT                                                                               | QIon  | Exp Ratio |
|------------------------------------------------------------------------------------|-------|--------------------------------------------------------------------------------------|-------|-----------|
| Chlorobenzene                                                                      | N.D.  | 9.80                                                                                 | 114.0 | 32.1      |
| + EIC (112.0) Scan 07JAN15.D                                                       |       | 112.0, 114.0                                                                         |       |           |
|    |       |    |       |           |
| 1,1,1,2-Tetrachloroethane                                                          | N.D.  | 9.89                                                                                 | 133.0 | 98.6      |
| + EIC (131.0) Scan 07JAN15.D                                                       |       | 131.0, 133.0                                                                         |       |           |
|   |       |   |       |           |
| Ethylbenzene                                                                       | N.D.  | 9.92                                                                                 | 106.0 | 31.1      |
| + EIC (91.0) Scan 07JAN15.D                                                        |       | 91.0, 106.0                                                                          |       |           |
|  |       |  |       |           |

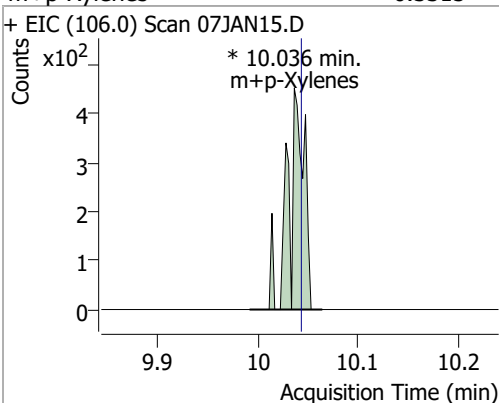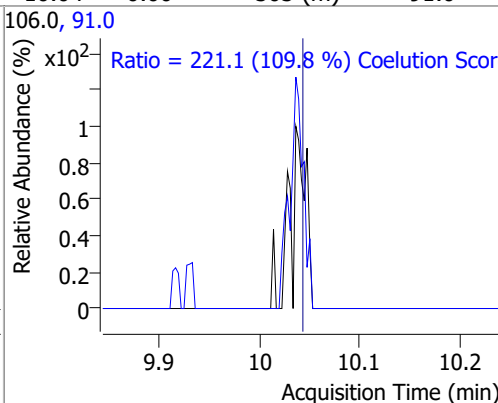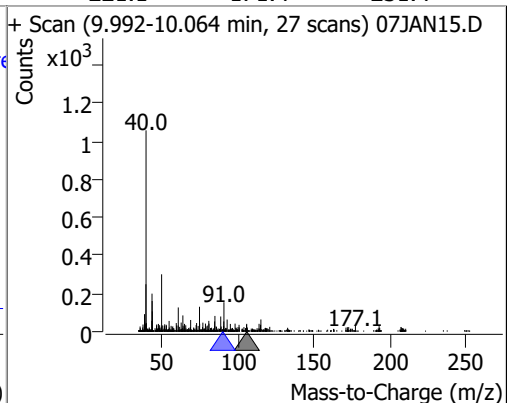
| Compound                                                                           | Conc.  | RT                                                                                   | Dev(Min) | Resp.   | QIon                                                                                  | QRatio | Lower | Upper |
|------------------------------------------------------------------------------------|--------|--------------------------------------------------------------------------------------|----------|---------|---------------------------------------------------------------------------------------|--------|-------|-------|
| m+p-Xylenes                                                                        | 0.3315 | 10.04                                                                                | 0.00     | 505 (m) | 91.0                                                                                  | 221.1  | 171.4 | 231.4 |
| + EIC (106.0) Scan 07JAN15.D                                                       |        | 106.0, 91.0                                                                          |          |         | Ratio = 221.1 (109.8 %) Coelution Score                                               |        |       |       |
|  |        |  |          |         |  |        |       |       |

# Quantitation Results Report (QT Reviewed)


| Compound | Conc. | RT | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|----------|-------|----|----------|-------|------|--------|-------|-------|
| o-Xylene |       | 0  |          | 0     | 91.0 |        | 183.1 | 243.1 |

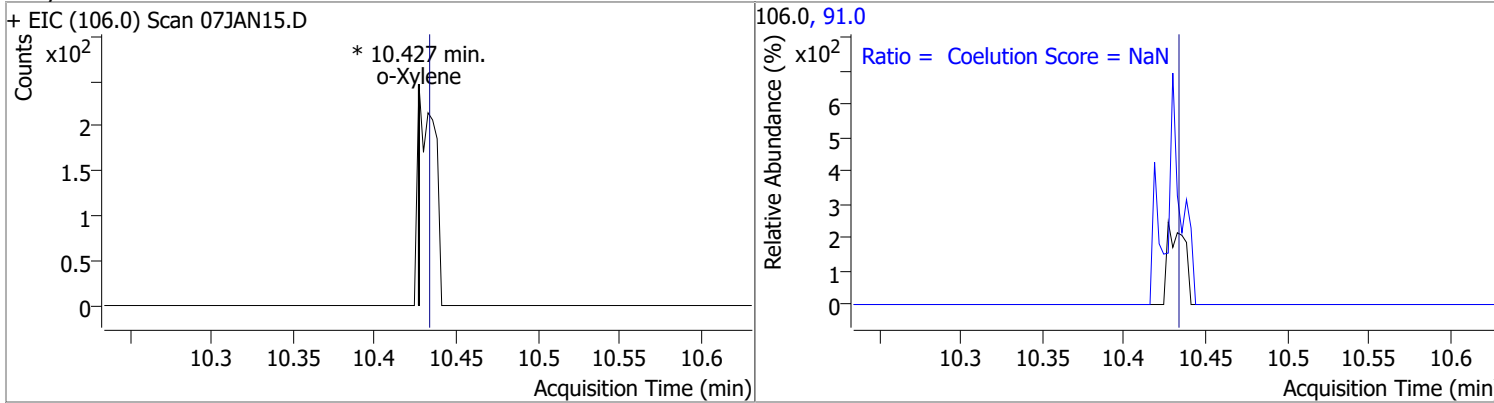


| Compound | Conc. | Exp RT | QIon | Exp Ratio |
|----------|-------|--------|------|-----------|
| Styrene  | N.D.  | 10.45  | 78.0 | 49.6      |

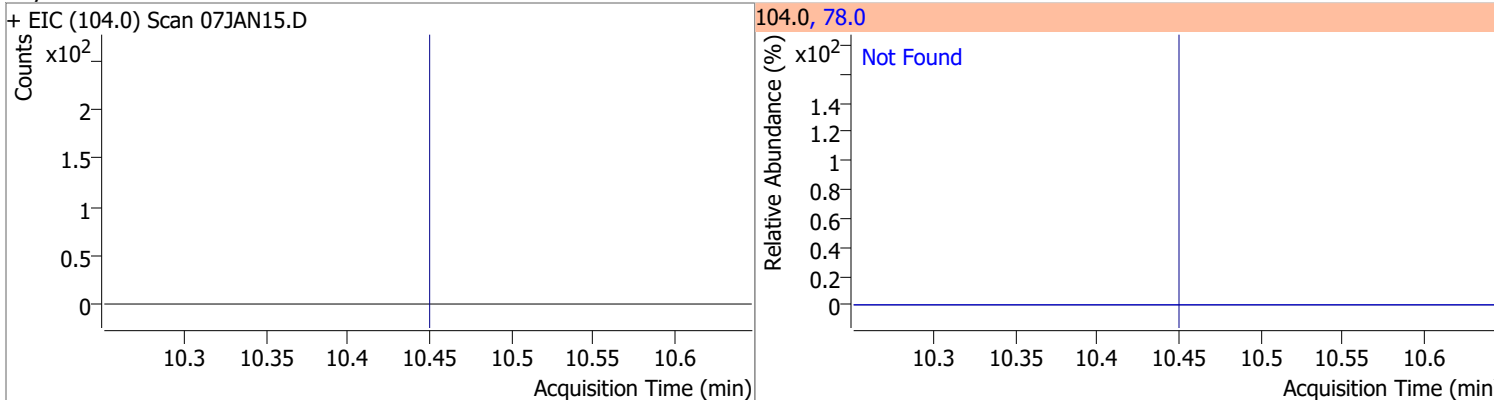









| Compound  | Conc. | Exp RT | QIon  | Exp Ratio | QIon  | Exp Ratio |
|-----------|-------|--------|-------|-----------|-------|-----------|
| Bromoform | N.D.  | 10.63  | 170.5 | 52.1      | 174.5 | 50.1      |

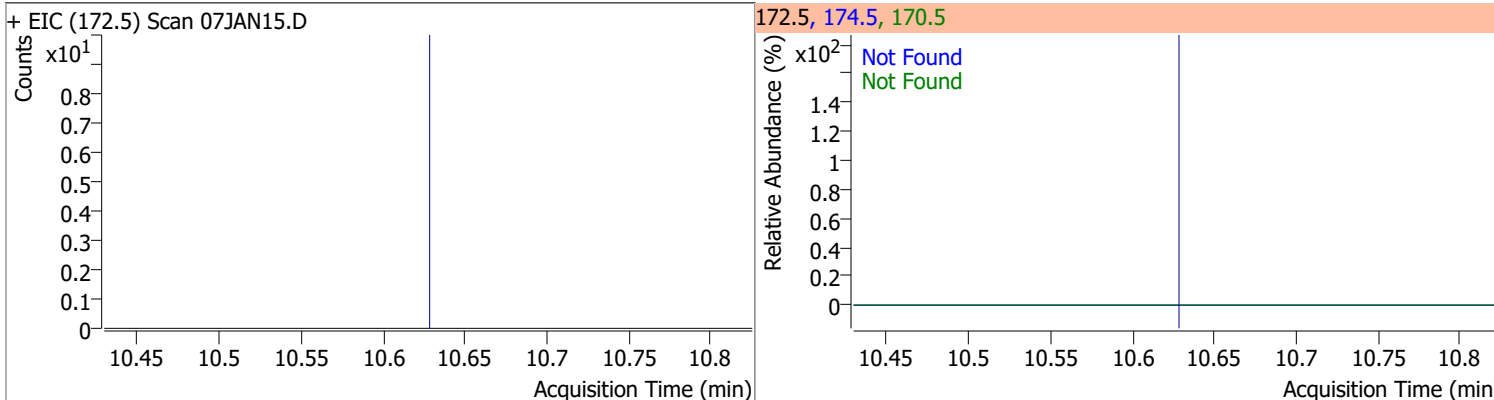









| Compound             | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 269.8409 | 10.95 | 0.00     | 240345 | 174.0 | 94.5   | 61.7  | 121.7 |
|                      |          |       |          |        | 176.0 | 91.5   | 60.6  | 120.6 |

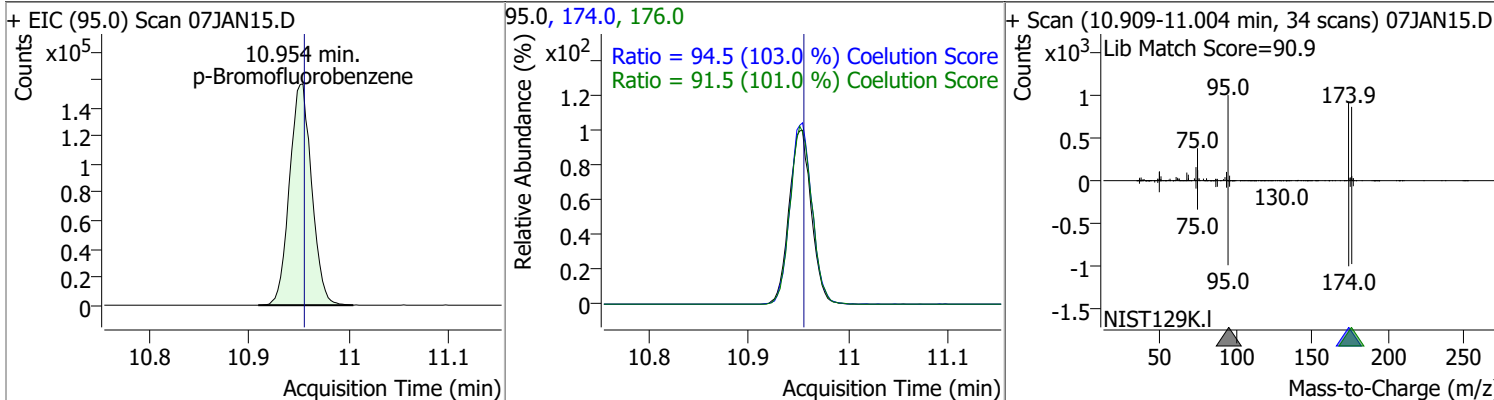

# Quantitation Results Report (QT Reviewed)

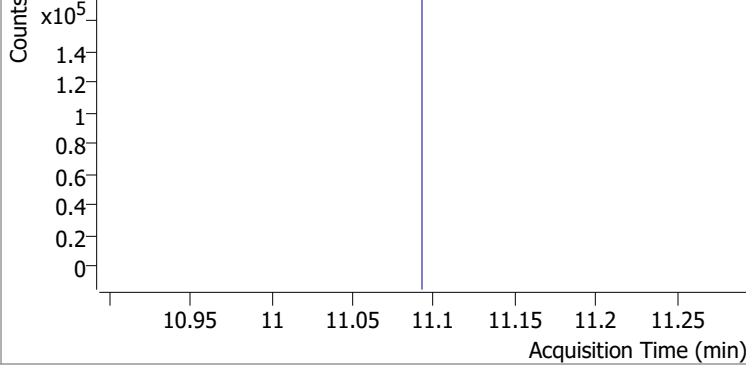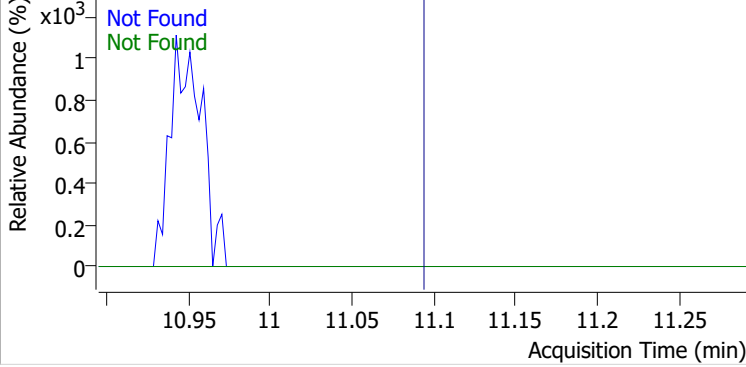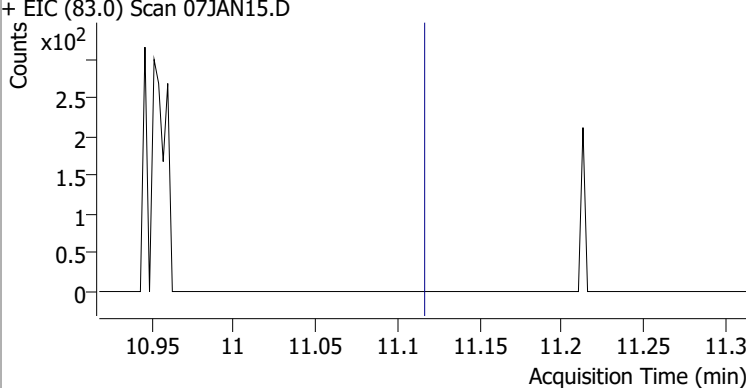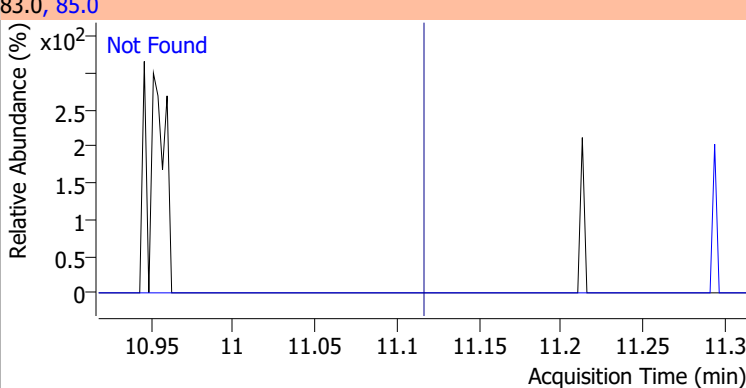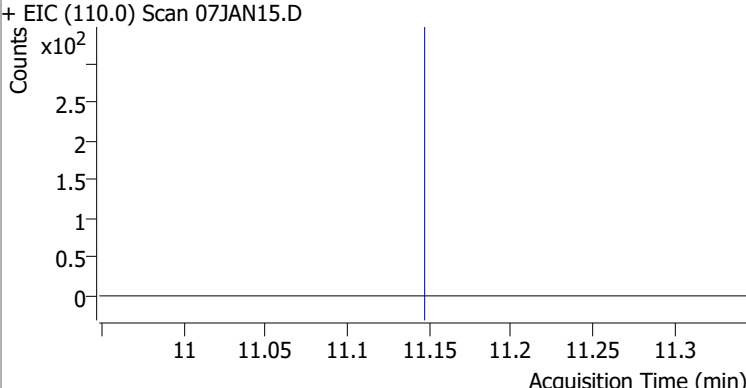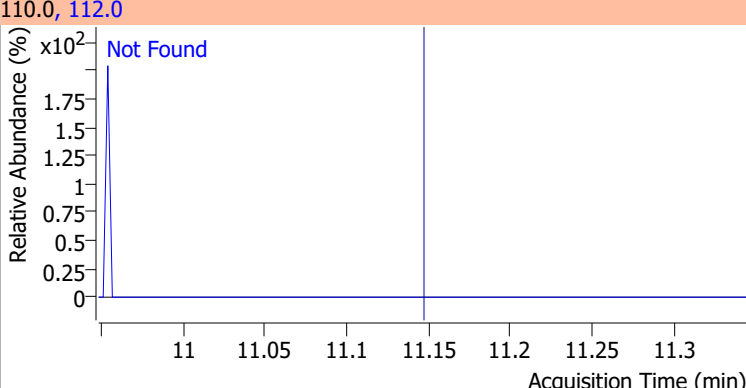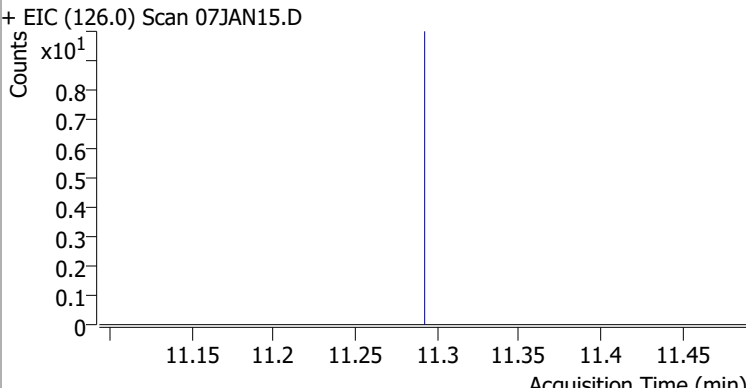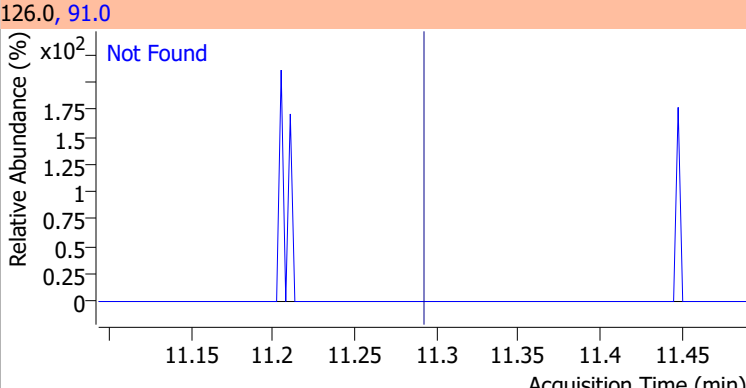
| Compound                                                                           | Conc. | Exp RT | QIon                                                                                 | Exp Ratio | QIon  | Exp Ratio |
|------------------------------------------------------------------------------------|-------|--------|--------------------------------------------------------------------------------------|-----------|-------|-----------|
| Bromobenzene                                                                       | N.D.  | 11.09  | 77.0                                                                                 | 145.7     | 158.0 | 96.5      |
| + EIC (156.0) Scan 07JAN15.D ***NO DATA POINTS***                                  |       |        | 156.0, 77.0, 158.0                                                                   |           |       |           |
|    |       |        |    |           |       |           |
| 1,1,2,2-Tetrachloroethane                                                          | N.D.  | 11.12  | 85.0                                                                                 | 66.2      |       |           |
| + EIC (83.0) Scan 07JAN15.D                                                        |       |        | 83.0, 85.0                                                                           |           |       |           |
|   |       |        |   |           |       |           |
| 1,2,3-Trichloropropane                                                             | N.D.  | 11.15  | 112.0                                                                                | 63.5      |       |           |
| + EIC (110.0) Scan 07JAN15.D                                                       |       |        | 110.0, 112.0                                                                         |           |       |           |
|  |       |        |  |           |       |           |
| 2-Chlorotoluene                                                                    | N.D.  | 11.29  | 91.0                                                                                 | 282.3     |       |           |
| + EIC (126.0) Scan 07JAN15.D                                                       |       |        | 126.0, 91.0                                                                          |           |       |           |
|  |       |        |  |           |       |           |

# Quantitation Results Report (QT Reviewed)
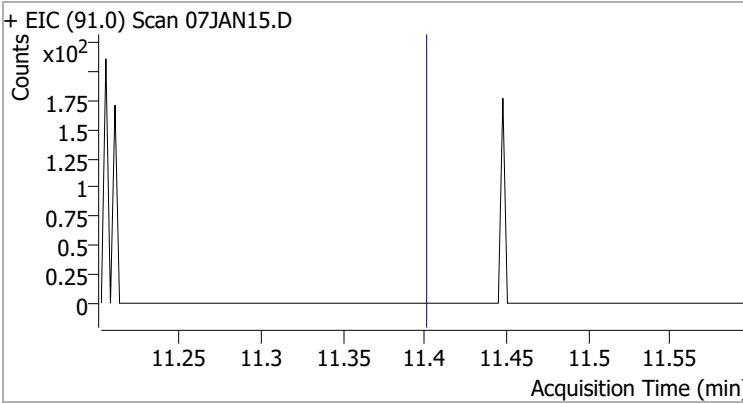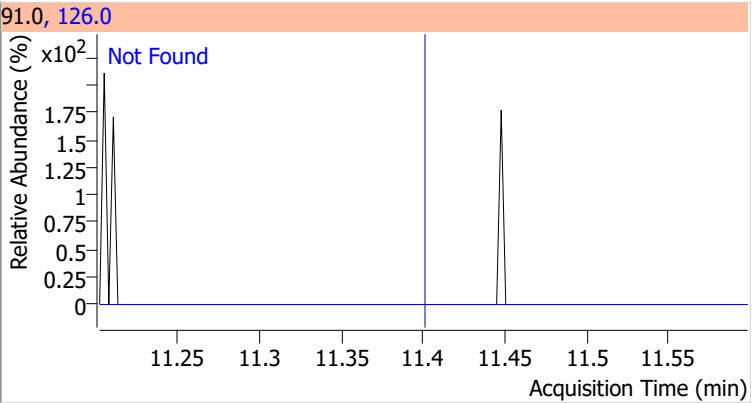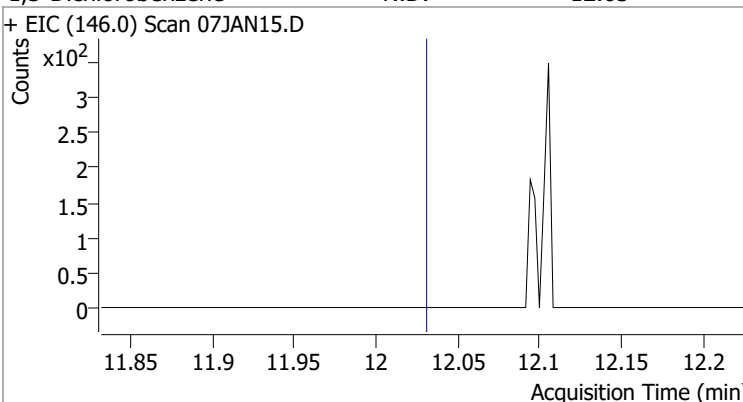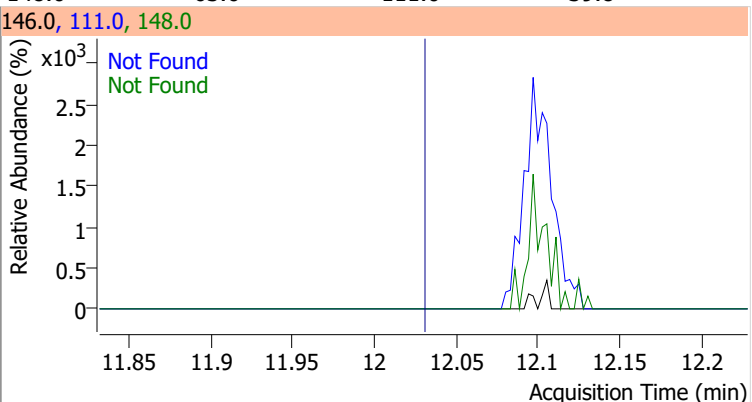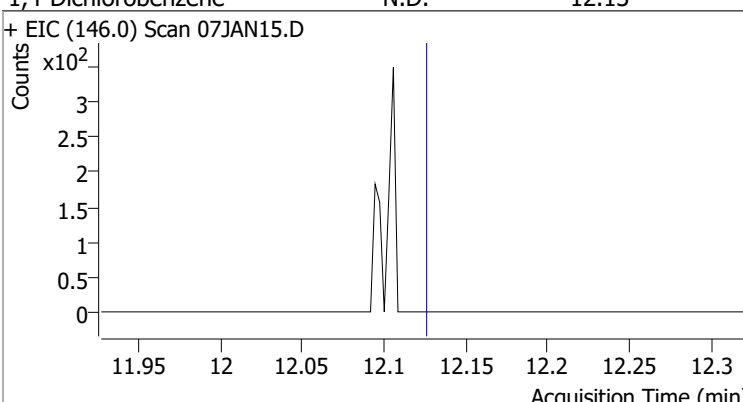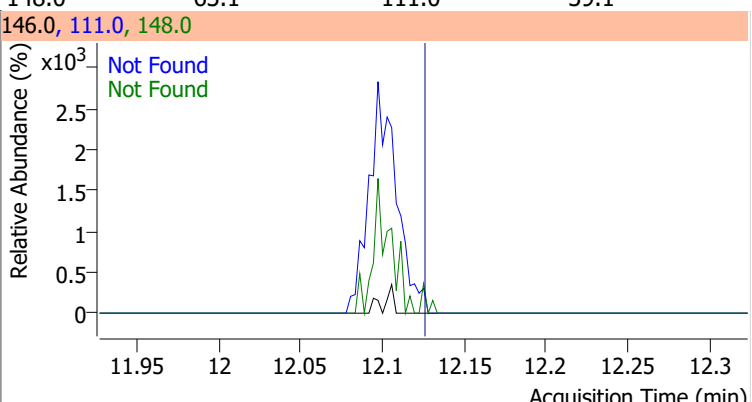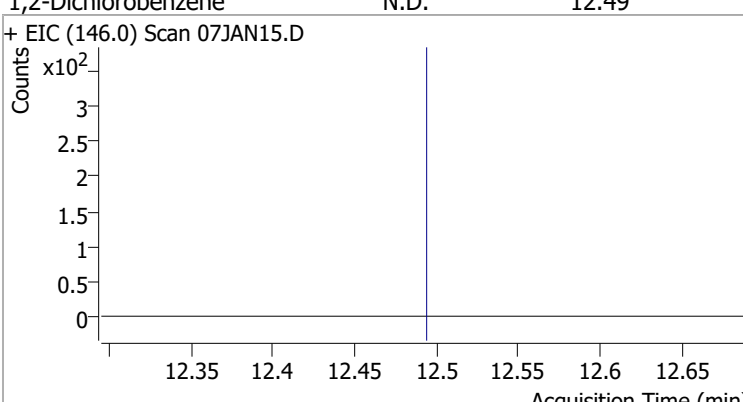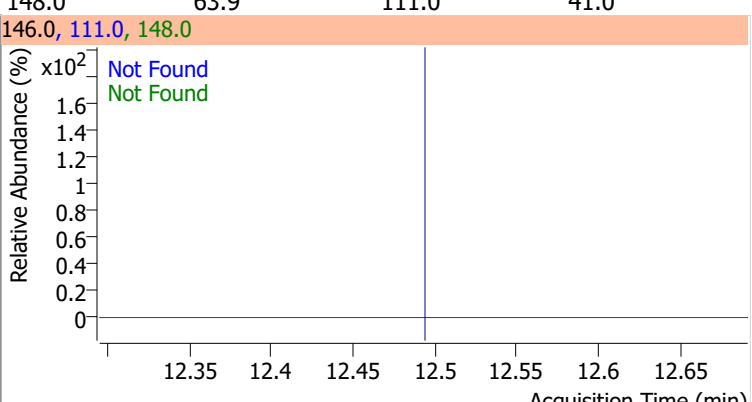
| Compound                                                                           | Conc. | Exp RT | QIon                                                                                 | Exp Ratio |      |           |
|------------------------------------------------------------------------------------|-------|--------|--------------------------------------------------------------------------------------|-----------|------|-----------|
| 4-Chlorotoluene                                                                    | N.D.  | 11.40  | 126.0                                                                                | 31.7      |      |           |
| + EIC (91.0) Scan 07JAN15.D                                                        |       |        | 91.0, 126.0                                                                          |           |      |           |
|    |       |        |    |           |      |           |
| 1,3-Dichlorobenzene                                                                | N.D.  | 12.03  | 148.0                                                                                | 63.6      | QIon | Exp Ratio |
| + EIC (146.0) Scan 07JAN15.D                                                       |       |        | 146.0, 111.0, 148.0                                                                  |           |      |           |
|   |       |        |   |           |      |           |
| 1,4-Dichlorobenzene                                                                | N.D.  | 12.13  | 148.0                                                                                | 63.1      | QIon | Exp Ratio |
| + EIC (146.0) Scan 07JAN15.D                                                       |       |        | 146.0, 111.0, 148.0                                                                  |           |      |           |
|  |       |        |  |           |      |           |
| 1,2-Dichlorobenzene                                                                | N.D.  | 12.49  | 148.0                                                                                | 63.9      | QIon | Exp Ratio |
| + EIC (146.0) Scan 07JAN15.D                                                       |       |        | 146.0, 111.0, 148.0                                                                  |           |      |           |
|  |       |        |  |           |      |           |

# Quantitation Results Report (QT Reviewed)

|                |                                     |                   |                       |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File      | 07JAN17.D                           | Operator          | MSC                   |
| Acq. Method    | 5975CACQF.M                         | Acq. Date-Time    | 1/7/2022 5:07:38 PM   |
| Sample Name    | B22010219-001FMS                    | Instrument        | VOA5975C              |
| Vial           | 17                                  | Multiplier        | 1.00                  |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m  | Comment           |                       |
| Tune File      | BFB_Atune3.u                        | Tune Date         | 10/11/2021 4:02:00 PM |
| Batch Name     | VG010722_8260B.batch.bin            | Last Calib Update | 3/2/2022 10:41:44 AM  |
| Ref Library    | \\MASSHUNTER\Org\Library\NIST129K.I |                   |                       |

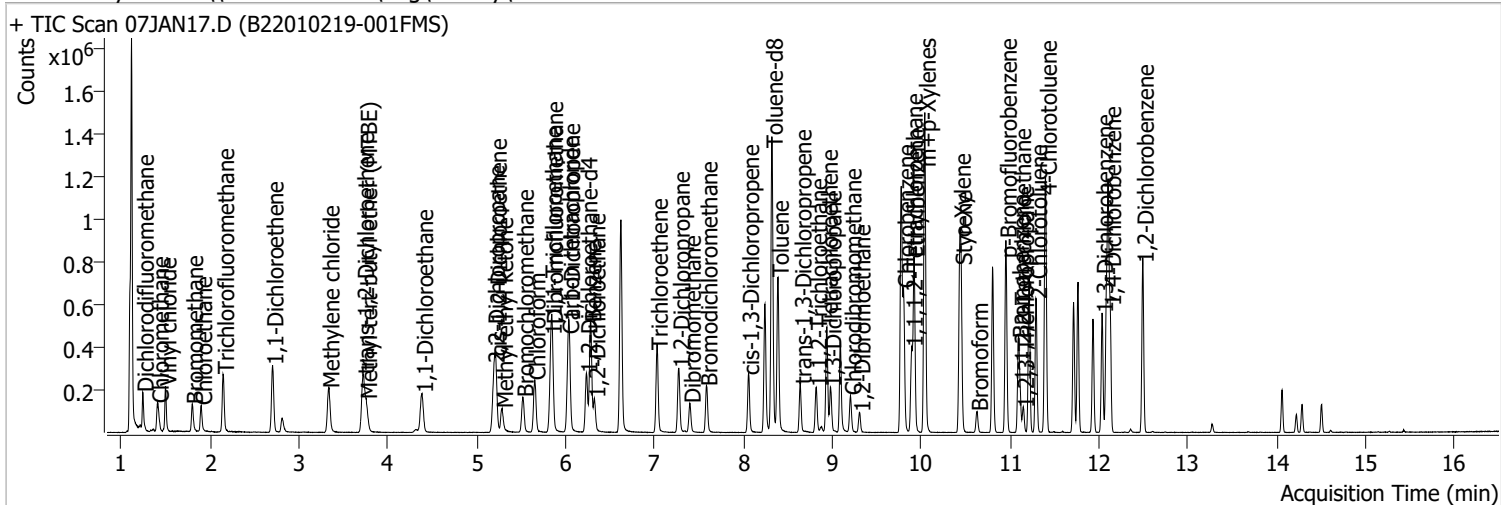

| Compound                           | RT                   | QIon  | Resp.              | Conc.     | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------------------|-----------|-------|----------|
| <b>Internal Standards</b>          |                      |       |                    |           |       |          |
| M Fluorobenzene                    | 6.620                | 96.0  | 855146             | 250.0000  | ng    | -0.003   |
| M Chlorobenzene-d5                 | 9.772                | 82.0  | 328555             | 250.0000  | ng    | 0.000    |
| M 1,4-Dichlorobenzene-d4           | 12.100               | 152.0 | 264037             | 250.0000  | ng    | 0.000    |
| <b>System Monitoring Compounds</b> |                      |       |                    |           |       |          |
| S Dibromofluoromethane             | 5.848                | 113.0 | 220360             | 273.5236  | ng    | 0.003    |
| Spiked Amount: 250.000             | Range: 80.0 - 119.0% |       | Recovery = 109.41% |           |       |          |
| S 1,2-Dichloroethane-d4            | 6.233                | 67.0  | 96662              | 277.7836  | ng    | 0.000    |
| Spiked Amount: 250.000             | Range: 81.0 - 118.0% |       | Recovery = 111.11% |           |       |          |
| S Toluene-d8                       | 8.319                | 98.0  | 860434             | 271.7626  | ng    | 0.000    |
| Spiked Amount: 250.000             | Range: 89.0 - 112.0% |       | Recovery = 108.71% |           |       |          |
| S p-Bromofluorobenzene             | 10.951               | 95.0  | 265093             | 274.0538  | ng    | -0.003   |
| Spiked Amount: 250.000             | Range: 85.0 - 114.0% |       | Recovery = 109.62% |           |       |          |
| <b>Target Compounds</b>            |                      |       |                    |           |       |          |
| T Dichlorodifluoromethane          | 1.241                | 85.0  | 120279             | 107.3334  | ng    | 99       |
| T Chloromethane                    | 1.411                | 50.0  | 152071             | 111.8049  | ng    | 99       |
| T Vinyl chloride                   | 1.498                | 62.0  | 150050             | 122.6032  | ng    | 97       |
| T Bromomethane                     | 1.799                | 96.0  | 66210              | 120.9860  | ng    | 98       |
| T Chloroethane                     | 1.899                | 64.0  | 85441              | 141.0182  | ng    | 97       |
| T Trichlorofluoromethane           | 2.145                | 101.0 | 189149             | 124.5150  | ng    | 98       |
| T 1,1-Dichloroethene               | 2.702                | 96.0  | 112908             | 131.0796  | ng    | 98       |
| T Methylene chloride               | 3.333                | 49.0  | 154851             | 121.9493  | ng    | 98       |
| T trans-1,2-Dichloroethene         | 3.720                | 96.0  | 114095             | 129.8323  | ng    | 98       |
| T Methyl tert-butyl ether (MTBE)   | 3.757                | 73.0  | 159167             | 140.1252  | ng    | 98       |
| T 1,1-Dichloroethane               | 4.384                | 63.0  | 221763             | 135.5713  | ng    | 98       |
| T 2,2-Dichloropropane              | 5.193                | 77.0  | 161563             | 131.8131  | ng    | 99       |
| T cis-1,2-Dichloroethene           | 5.212                | 96.0  | 116966             | 131.2799  | ng    | 97       |
| T Methyl ethyl ketone              | 5.285                | 43.0  | 151656             | 1256.6341 | ng    | 100      |
| T Bromochloromethane               | 5.516                | 128.0 | 45934              | 124.4477  | ng    | 94       |
| T Chloroform                       | 5.650                | 83.0  | 197751             | 121.4742  | ng    | 98       |















# Quantitation Results Report (QT Reviewed)

| Compound                    | RT     | QIon  | Resp.  | Conc.    | Units | Dev(Min) |
|-----------------------------|--------|-------|--------|----------|-------|----------|
| T 1,1,1-Trichloroethane     | 5.831  | 97.0  | 190350 | 124.7685 | ng    | 98       |
| T Carbon tetrachloride      | 6.026  | 117.0 | 182925 | 121.6947 | ng    | 98       |
| T 1,1-Dichloropropene       | 6.038  | 75.0  | 157497 | 121.4151 | ng    | 100      |
| T Benzene                   | 6.280  | 78.0  | 443412 | 130.2309 | ng    | 100      |
| T 1,2-Dichloroethane        | 6.322  | 62.0  | 117773 | 127.8627 | ng    | 98       |
| T Trichloroethene           | 7.025  | 95.0  | 124303 | 125.4471 | ng    | 98       |
| T 1,2-Dichloropropane       | 7.273  | 63.0  | 109245 | 125.3364 | ng    | 100      |
| T Dibromomethane            | 7.396  | 93.0  | 46329  | 125.7798 | ng    | 97       |
| T Bromodichloromethane      | 7.583  | 83.0  | 130361 | 128.2418 | ng    | 99       |
| T cis-1,3-Dichloropropene   | 8.054  | 75.0  | 139124 | 121.0494 | ng    | 99       |
| T Toluene                   | 8.386  | 92.0  | 276475 | 129.2716 | ng    | 99       |
| T trans-1,3-Dichloropropene | 8.639  | 75.0  | 108385 | 132.4832 | ng    | 97       |
| T 1,1,2-Trichloroethane     | 8.818  | 83.0  | 52652  | 123.5591 | ng    | 96       |
| T Tetrachloroethene         | 8.938  | 163.8 | 106788 | 122.3903 | ng    | 99       |
| T 1,3-Dichloropropane       | 8.980  | 76.0  | 106245 | 126.7568 | ng    | 96       |
| T Chlorodibromomethane      | 9.203  | 129.0 | 83355  | 125.1595 | ng    | 96       |
| T 1,2-Dibromoethane         | 9.303  | 107.0 | 58167  | 124.8389 | ng    | 100      |
| T Chlorobenzene             | 9.799  | 112.0 | 300347 | 128.2720 | ng    | 100      |
| T 1,1,1,2-Tetrachloroethane | 9.892  | 131.0 | 101471 | 123.9720 | ng    | 96       |
| T Ethylbenzene              | 9.917  | 91.0  | 515970 | 127.0574 | ng    | 100      |
| T m+p-Xylenes               | 10.039 | 106.0 | 399658 | 253.2483 | ng    | 100      |
| T o-Xylene                  | 10.433 | 106.0 | 183667 | 130.7338 | ng    | 98       |
| T Styrene                   | 10.449 | 104.0 | 299523 | 132.4202 | ng    | 100      |
| T Bromoform                 | 10.628 | 172.5 | 43824  | 129.7036 | ng    | 98       |
| T Bromobenzene              | 11.091 | 156.0 | 114173 | 133.6149 | ng    | 99       |
| T 1,1,2,2-Tetrachloroethane | 11.110 | 83.0  | 64543  | 131.2329 | ng    | 97       |
| T 1,2,3-Trichloropropane    | 11.144 | 110.0 | 16295  | 123.8246 | ng    | 98       |
| T 2-Chlorotoluene           | 11.291 | 126.0 | 111645 | 131.3133 | ng    | 99       |
| T 4-Chlorotoluene           | 11.400 | 91.0  | 369533 | 133.3048 | ng    | 99       |
| T 1,3-Dichlorobenzene       | 12.033 | 146.0 | 204772 | 131.3970 | ng    | 99       |
| T 1,4-Dichlorobenzene       | 12.125 | 146.0 | 206411 | 129.8964 | ng    | 99       |
| T 1,2-Dichlorobenzene       | 12.493 | 146.0 | 165895 | 125.9590 | ng    | 99       |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (\*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

# Quantitation Results Report (QT Reviewed)

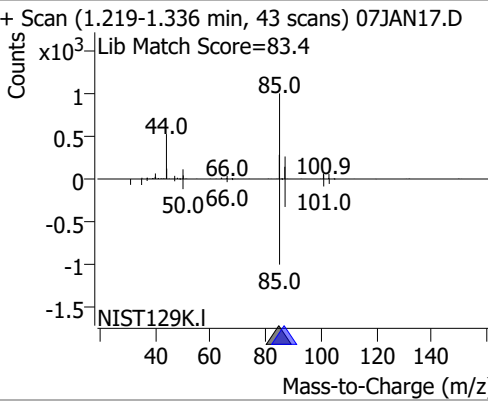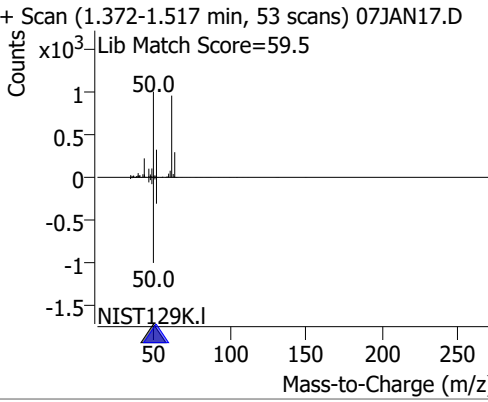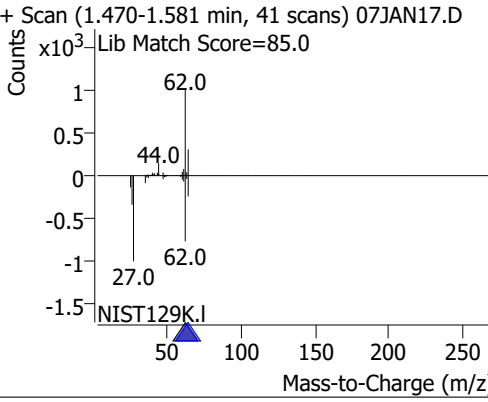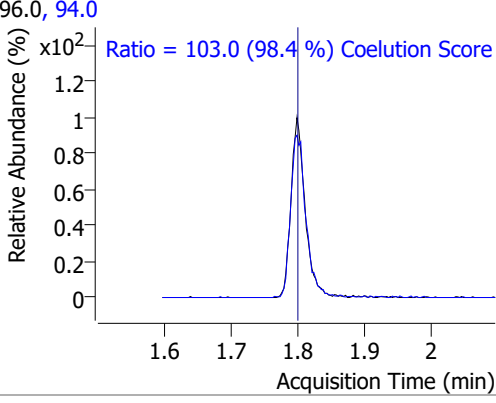
| Compound                                                                           | Conc.                                                                                | RT                                                                                    | Dev(Min)   | Resp.  | QIon | QRatio                                       | Lower | Upper |
|------------------------------------------------------------------------------------|--------------------------------------------------------------------------------------|---------------------------------------------------------------------------------------|------------|--------|------|----------------------------------------------|-------|-------|
| Dichlorodifluoromethane                                                            | 107.3334                                                                             | 1.24                                                                                  | 0.00       | 120279 | 87.0 | 31.7                                         | 2.3   | 62.3  |
| + EIC (85.0) Scan 07JAN17.D                                                        |                                                                                      |                                                                                       | 85.0, 87.0 |        |      | + Scan (1.219-1.336 min, 43 scans) 07JAN17.D |       |       |
|    |    |    |            |        |      |                                              |       |       |
| Chloromethane                                                                      | 111.8049                                                                             | 1.41                                                                                  | 0.00       | 152071 | 52.0 | 32.7                                         | 2.1   | 62.1  |
| + EIC (50.0) Scan 07JAN17.D                                                        |                                                                                      |                                                                                       | 50.0, 52.0 |        |      | + Scan (1.372-1.517 min, 53 scans) 07JAN17.D |       |       |
|   |   |   |            |        |      |                                              |       |       |
| Vinyl chloride                                                                     | 122.6032                                                                             | 1.50                                                                                  | 0.00       | 150050 | 64.0 | 31.3                                         | 0.0   | 59.9  |
| + EIC (62.0) Scan 07JAN17.D                                                        |                                                                                      |                                                                                       | 62.0, 64.0 |        |      | + Scan (1.470-1.581 min, 41 scans) 07JAN17.D |       |       |
|  |  |  |            |        |      |                                              |       |       |
| Bromomethane                                                                       | 120.9860                                                                             | 1.80                                                                                  | 0.00       | 66210  | 94.0 | 103.0                                        | 74.6  | 134.6 |
| + EIC (96.0) Scan 07JAN17.D                                                        |                                                                                      |                                                                                       | 96.0, 94.0 |        |      | + Scan (1.765-1.877 min, 40 scans) 07JAN17.D |       |       |
|  |  |  |            |        |      |                                              |       |       |

# Quantitation Results Report (QT Reviewed)


| Compound     | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|----------|------|----------|-------|------|--------|-------|-------|
| Chloroethane | 141.0182 | 1.90 | 0.01     | 85441 | 66.0 | 31.6   | 0.1   | 60.1  |




|                        |          |      |      |        |       |      |      |      |
|------------------------|----------|------|------|--------|-------|------|------|------|
| Trichlorofluoromethane | 124.5150 | 2.14 | 0.00 | 189149 | 103.0 | 65.9 | 34.2 | 94.2 |
|------------------------|----------|------|------|--------|-------|------|------|------|



|                    |          |      |      |        |      |       |       |       |
|--------------------|----------|------|------|--------|------|-------|-------|-------|
| 1,1-Dichloroethene | 131.0796 | 2.70 | 0.01 | 112908 | 61.0 | 177.0 | 150.3 | 210.3 |
|                    |          |      |      |        | 63.0 | 56.2  | 26.7  | 86.7  |




|                    |          |      |      |        |      |      |      |      |
|--------------------|----------|------|------|--------|------|------|------|------|
| Methylene chloride | 121.9493 | 3.33 | 0.00 | 154851 | 84.0 | 67.2 | 36.9 | 96.9 |
|                    |          |      |      |        | 86.0 | 41.8 | 14.3 | 74.3 |




# Quantitation Results Report (QT Reviewed)


| Compound                 | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------------|----------|------|----------|--------|------|--------|-------|-------|
| trans-1,2-Dichloroethene | 129.8323 | 3.72 | 0.00     | 114095 | 61.0 | 156.1  | 123.9 | 183.9 |
|                          |          |      |          |        | 98.0 | 64.0   | 35.7  | 95.7  |

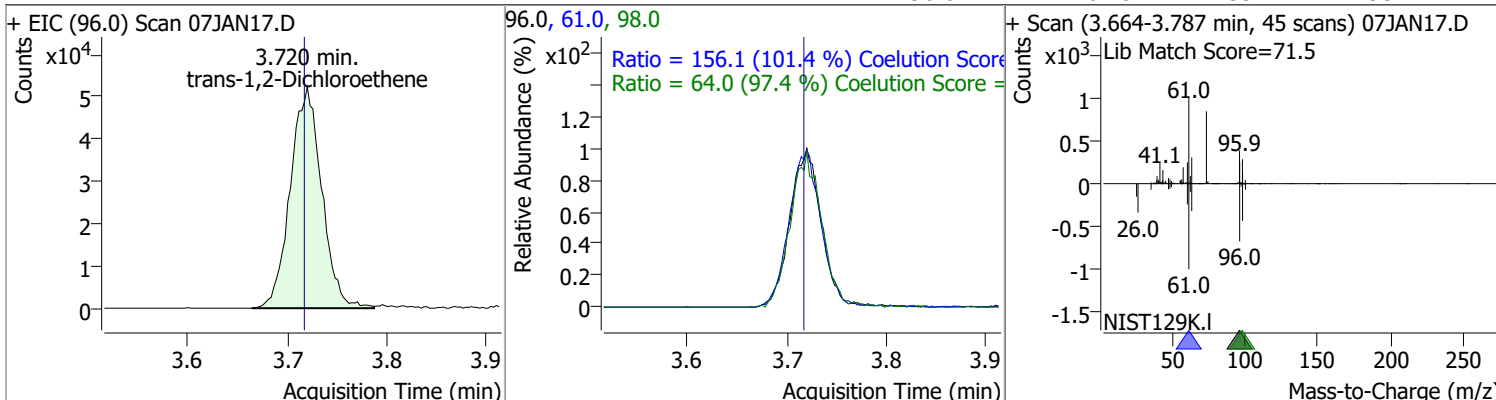

| Compound                       | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------------------|----------|------|----------|--------|------|--------|-------|-------|
| Methyl tert-butyl ether (MTBE) | 140.1252 | 3.76 | 0.00     | 159167 | 57.0 | 25.6   | 0.0   | 54.6  |




| Compound           | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1-Dichloroethane | 135.5713 | 4.38 | 0.01     | 221763 | 65.0 | 31.2   | 2.1   | 62.1  |
|                    |          |      |          |        | 83.0 | 12.8   | 0.0   | 43.7  |




# Quantitation Results Report (QT Reviewed)


| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 2,2-Dichloropropane | 131.8131 | 5.19 | 0.00     | 161563 | 41.0 | 67.2   | 36.5  | 96.5  |
|                     |          |      |          |        | 97.0 | 23.4   | 0.0   | 53.2  |




| Compound               | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,2-Dichloroethene | 131.2799 | 5.21 | 0.00     | 116966 | 61.0 | 163.2  | 137.2 | 197.2 |
|                        |          |      |          |        | 98.0 | 65.2   | 37.3  | 97.3  |



| Compound            | Conc.     | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|-----------|------|----------|--------|------|--------|-------|-------|
| Methyl ethyl ketone | 1256.6341 | 5.28 | 0.00     | 151656 | 72.0 | 21.1   | 0.0   | 51.3  |




| Compound           | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|-------|------|--------|-------|-------|
| Bromochloromethane | 124.4477 | 5.52 | 0.00     | 45934 | 49.0 | 191.3  | 152.9 | 212.9 |




# Quantitation Results Report (QT Reviewed)


| Compound   | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|------|--------|-------|-------|
| Chloroform | 121.4742 | 5.65 | 0.00     | 197751 | 85.0 | 64.4   | 36.0  | 96.0  |

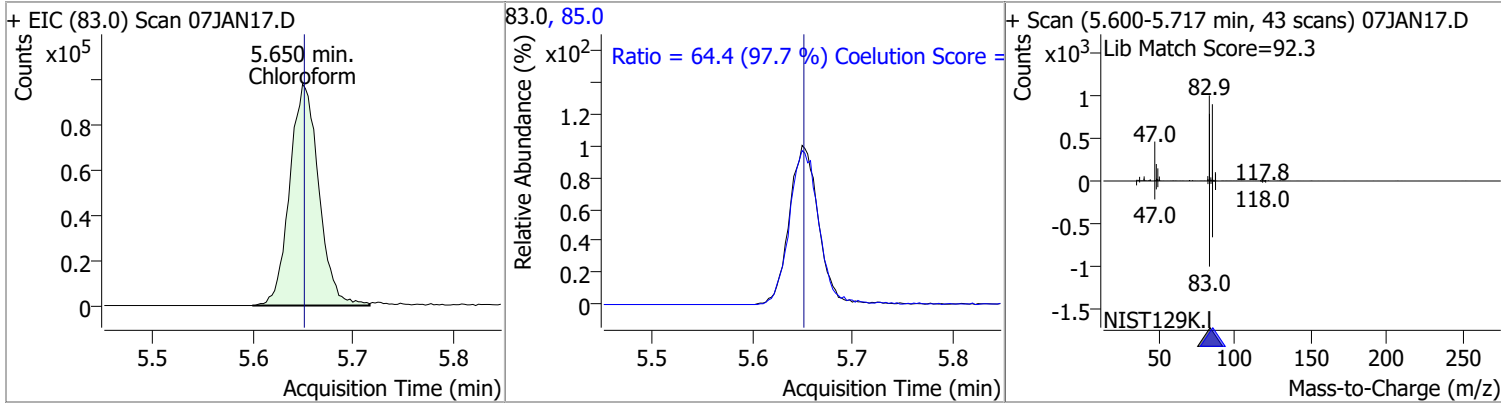


|                       |          |      |      |        |      |      |      |      |
|-----------------------|----------|------|------|--------|------|------|------|------|
| 1,1,1-Trichloroethane | 124.7685 | 5.83 | 0.00 | 190350 | 99.0 | 62.8 | 34.7 | 94.7 |
|                       |          |      |      |        | 61.0 | 48.7 | 18.1 | 78.1 |

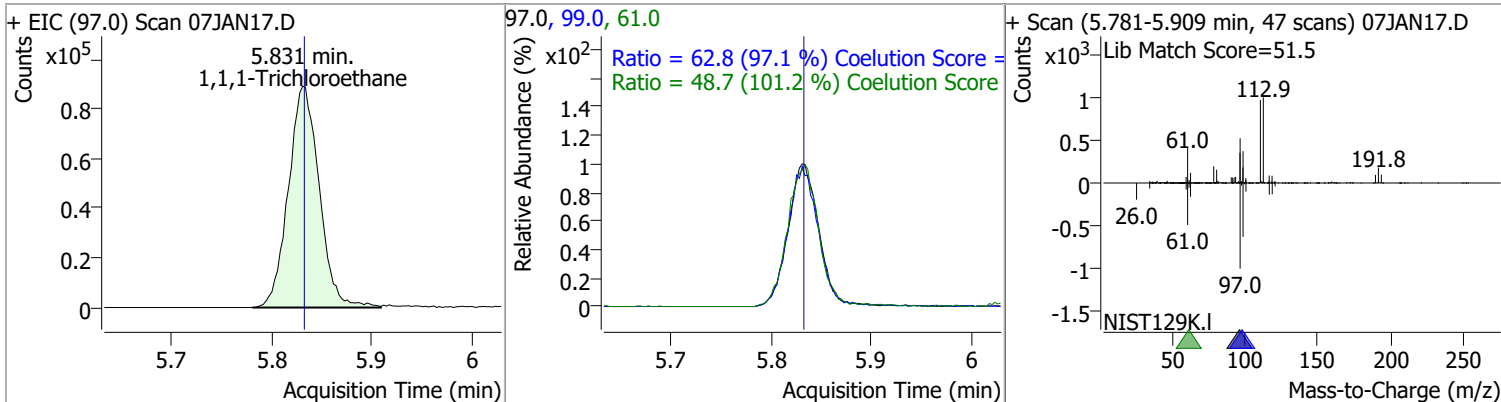

|                      |          |      |      |        |       |      |     |      |
|----------------------|----------|------|------|--------|-------|------|-----|------|
| Dibromofluoromethane | 273.5236 | 5.85 | 0.00 | 220360 | 191.5 | 21.6 | 0.0 | 53.1 |
|----------------------|----------|------|------|--------|-------|------|-----|------|

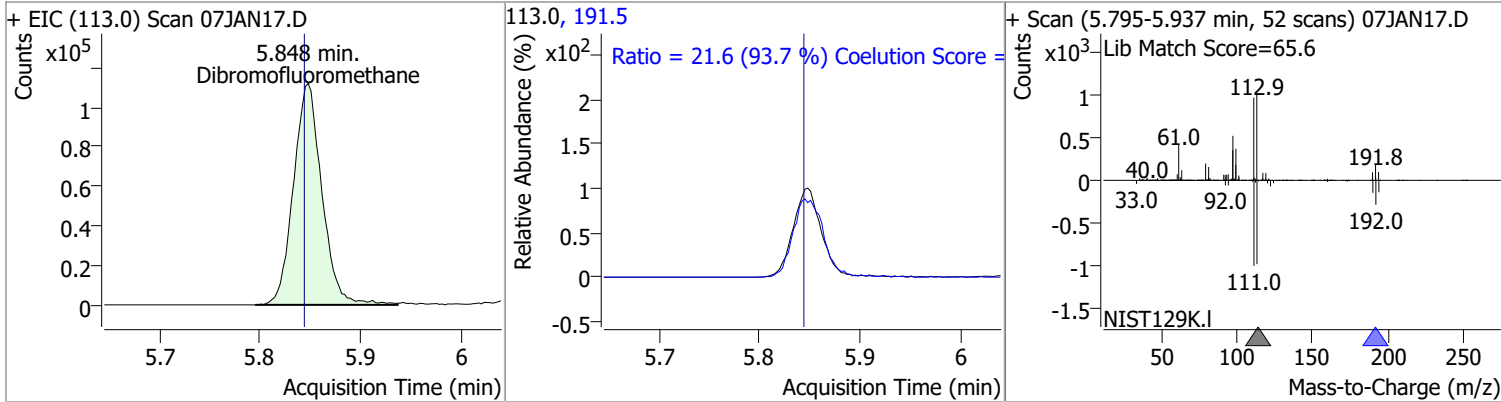


|                      |          |      |      |        |       |      |      |       |
|----------------------|----------|------|------|--------|-------|------|------|-------|
| Carbon tetrachloride | 121.6947 | 6.03 | 0.00 | 182925 | 119.0 | 95.5 | 67.2 | 127.2 |
|                      |          |      |      |        | 121.0 | 29.6 | 0.1  | 60.1  |

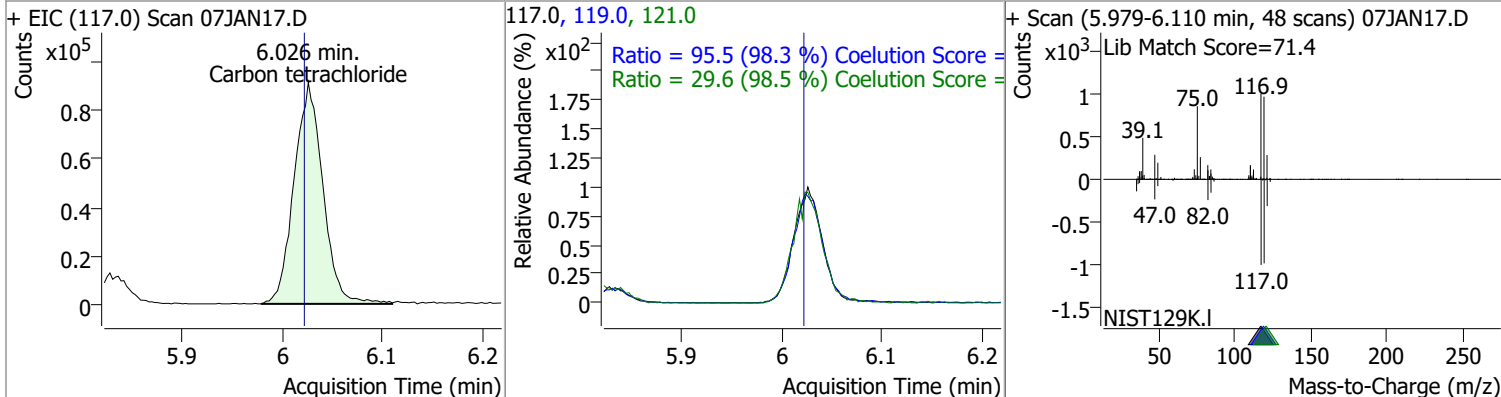


# Quantitation Results Report (QT Reviewed)


| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|-------|--------|-------|-------|
| 1,1-Dichloropropene | 121.4151 | 6.04 | 0.00     | 157497 | 110.0 | 35.7   | 5.9   | 65.9  |
|                     |          |      |          |        | 77.0  | 30.3   | 0.1   | 60.1  |




| Compound              | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio                                    | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|-------------------------------------------|-------|-------|
| 1,2-Dichloroethane-d4 | 277.7836 | 6.23 | 0.00     | 96662 | 65.0 | 199.5                                     | 166.5 | 226.5 |
|                       |          |      |          |       | 67.0 | Ratio = 199.5 (101.5 %) Coelution Score = |       |       |



| Compound | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio                                  | Lower | Upper |
|----------|----------|------|----------|--------|------|-----------------------------------------|-------|-------|
| Benzene  | 130.2309 | 6.28 | 0.00     | 443412 | 77.0 | 23.4                                    | 0.0   | 53.5  |
|          |          |      |          |        | 78.0 | Ratio = 23.4 (99.5 %) Coelution Score = |       |       |




| Compound           | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio                                   | Lower | Upper |
|--------------------|----------|------|----------|--------|------|------------------------------------------|-------|-------|
| 1,2-Dichloroethane | 127.8627 | 6.32 | 0.00     | 117773 | 64.0 | 31.1                                     | 0.0   | 59.9  |
|                    |          |      |          |        | 98.0 | 7.2                                      | 0.0   | 37.6  |
|                    |          |      |          |        | 62.0 | Ratio = 31.1 (104.0 %) Coelution Score = |       |       |




# Quantitation Results Report (QT Reviewed)


| Compound        | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|-----------------|----------|------|----------|--------|-------|--------|-------|-------|
| Trichloroethene | 125.4471 | 7.02 | -0.01    | 124303 | 130.0 | 103.6  | 71.5  | 131.5 |
|                 |          |      |          |        | 97.0  | 66.3   | 34.1  | 94.1  |



| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloropropane | 125.3364 | 7.27 | 0.00     | 109245 | 76.0 | 38.4   | 8.2   | 68.2  |




| Compound       | Conc.    | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|----------------|----------|------|----------|-------|-------|--------|-------|-------|
| Dibromomethane | 125.7798 | 7.40 | 0.00     | 46329 | 173.5 | 109.7  | 83.7  | 143.7 |
|                |          |      |          |       | 95.0  | 83.7   | 52.2  | 112.2 |






# Quantitation Results Report (QT Reviewed)


| Compound             | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Bromodichloromethane | 128.2418 | 7.58 | 0.00     | 130361 | 85.0  | 65.7   | 34.5  | 94.5  |
|                      |          |      |          |        | 127.0 | 9.2    | 0.0   | 39.6  |












| Compound                | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|-------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,3-Dichloropropene | 121.0494 | 8.05 | -0.01    | 139124 | 39.0 | 53.9   | 23.3  | 83.3  |
|                         |          |      |          |        | 77.0 | 31.6   | 1.0   | 61.0  |



| Compound   | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 271.7626 | 8.32 | 0.00     | 860434 | 100.0 | 64.6   | 34.4  | 94.4  |
|            |          |      |          |        | 99.0  | 9.6    | 0.0   | 39.6  |




# Quantitation Results Report (QT Reviewed)

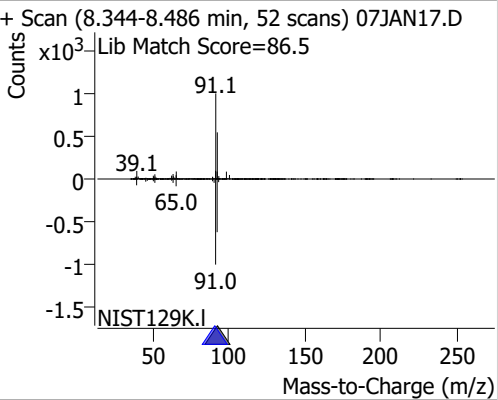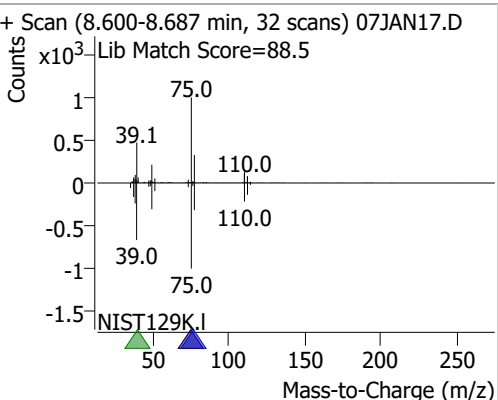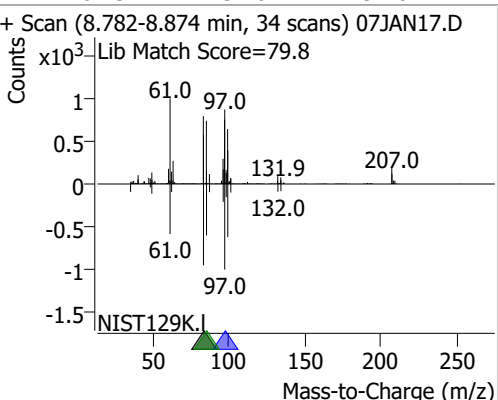
| Compound                                                                           | Conc.    | RT   | Dev(Min)                                                                             | Resp.  | QIon | QRatio                                                                                | Lower | Upper |
|------------------------------------------------------------------------------------|----------|------|--------------------------------------------------------------------------------------|--------|------|---------------------------------------------------------------------------------------|-------|-------|
| Toluene                                                                            | 129.2716 | 8.39 | 0.00                                                                                 | 276475 | 91.0 | 173.7                                                                                 | 145.8 | 205.8 |
| + EIC (92.0) Scan 07JAN17.D                                                        |          |      | 92.0, 91.0                                                                           |        |      | + Scan (8.344-8.486 min, 52 scans) 07JAN17.D                                          |       |       |
|    |          |      |    |        |      |    |       |       |
| trans-1,3-Dichloropropene                                                          | 132.4832 | 8.64 | 0.00                                                                                 | 108385 | 39.0 | 50.1                                                                                  | 23.4  | 83.4  |
| + EIC (75.0) Scan 07JAN17.D                                                        |          |      | 75.0, 77.0, 39.0                                                                     |        |      | + Scan (8.600-8.687 min, 32 scans) 07JAN17.D                                          |       |       |
|   |          |      |   |        |      |   |       |       |
| 1,1,2-Trichloroethane                                                              | 123.5591 | 8.82 | 0.00                                                                                 | 52652  | 97.0 | 118.4                                                                                 | 84.6  | 144.6 |
| + EIC (83.0) Scan 07JAN17.D                                                        |          |      | 83.0, 97.0, 85.0                                                                     |        |      | + Scan (8.782-8.874 min, 34 scans) 07JAN17.D                                          |       |       |
|  |          |      |  |        |      |  |       |       |

# Quantitation Results Report (QT Reviewed)


| Compound          | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|-------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Tetrachloroethene | 122.3903 | 8.94 | 0.00     | 106788 | 165.8 | 127.3  | 98.6  | 158.6 |
|                   |          |      |          |        | 129.0 | 90.8   | 61.5  | 121.5 |

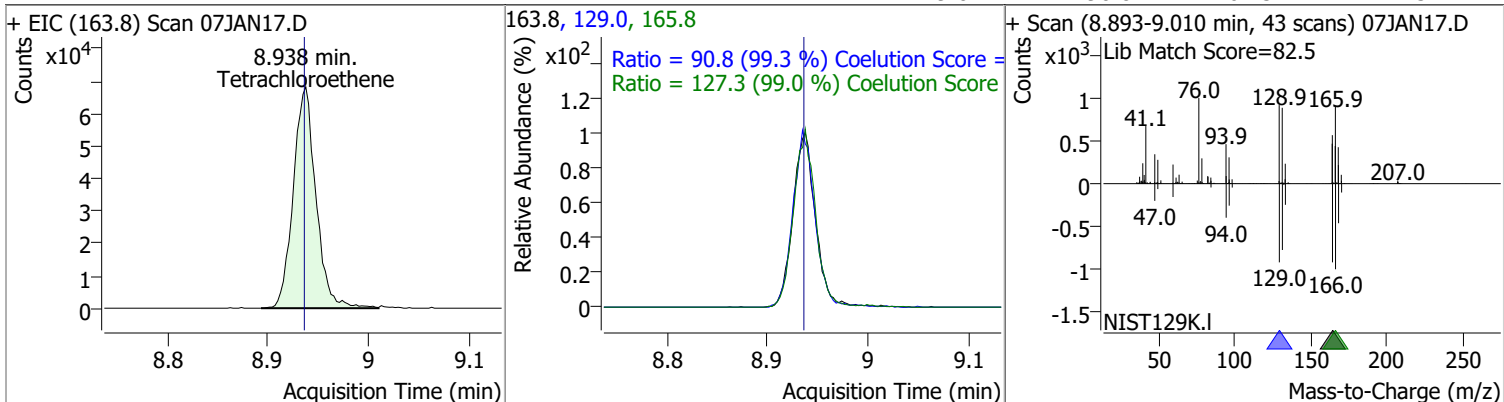


| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,3-Dichloropropane | 126.7568 | 8.98 | 0.00     | 106245 | 78.0 | 30.8   | 2.9   | 62.9  |

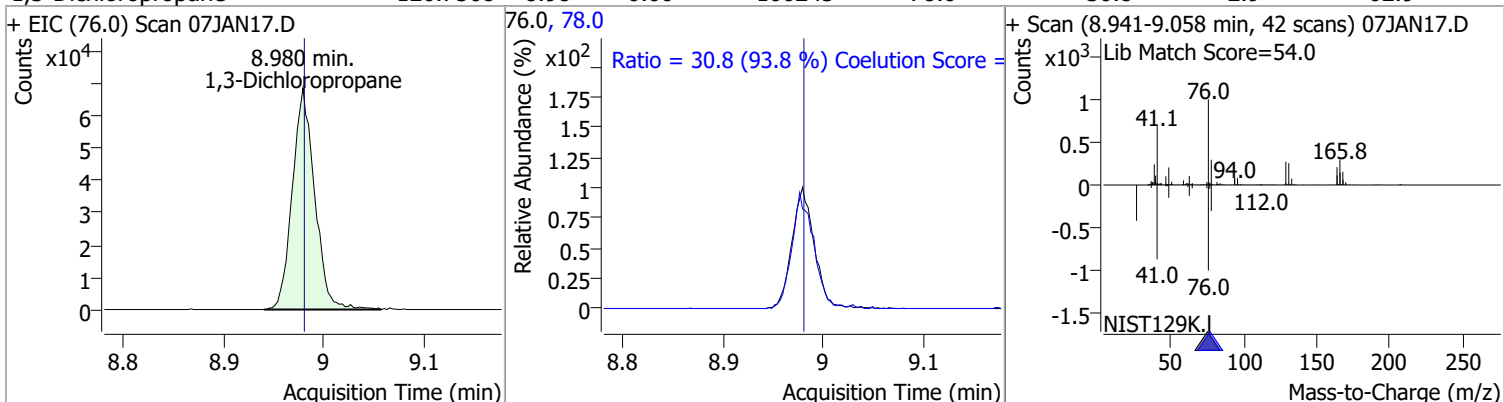

| Compound             | Conc.    | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|----------------------|----------|------|----------|-------|-------|--------|-------|-------|
| Chlorodibromomethane | 125.1595 | 9.20 | 0.00     | 83355 | 127.0 | 74.9   | 48.0  | 108.0 |




| Compound          | Conc.    | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|-------------------|----------|------|----------|-------|-------|--------|-------|-------|
| 1,2-Dibromoethane | 124.8389 | 9.30 | 0.00     | 58167 | 109.0 | 94.8   | 64.5  | 124.5 |




# Quantitation Results Report (QT Reviewed)


| Compound      | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|---------------|----------|------|----------|--------|-------|--------|-------|-------|
| Chlorobenzene | 128.2720 | 9.80 | 0.00     | 300347 | 114.0 | 32.0   | 2.1   | 62.1  |

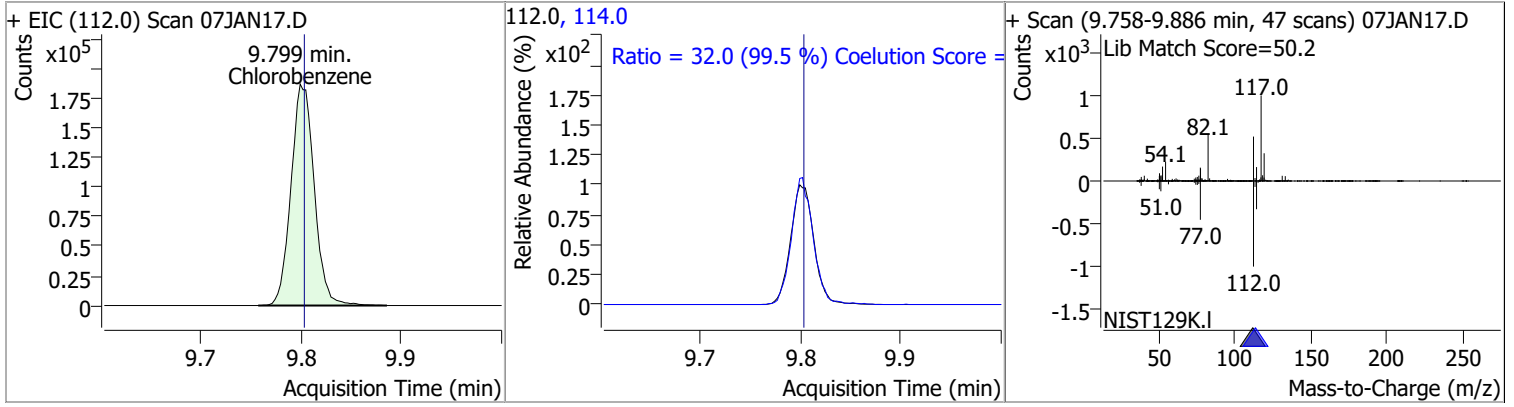


| Compound                  | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|---------------------------|----------|------|----------|--------|-------|--------|-------|-------|
| 1,1,1,2-Tetrachloroethane | 123.9720 | 9.89 | 0.00     | 101471 | 133.0 | 95.1   | 68.6  | 128.6 |

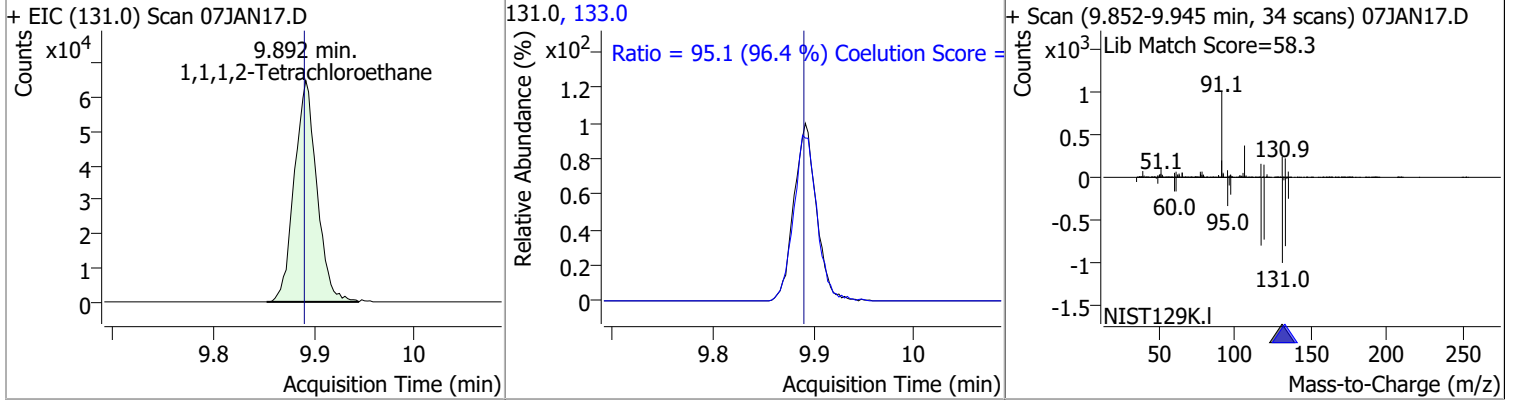





| Compound     | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|--------------|----------|------|----------|--------|-------|--------|-------|-------|
| Ethylbenzene | 127.0574 | 9.92 | 0.00     | 515970 | 106.0 | 31.1   | 1.1   | 61.1  |















| Compound    | Conc.    | RT    | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|-------------|----------|-------|----------|--------|------|--------|-------|-------|
| m+p-Xylenes | 253.2483 | 10.04 | 0.00     | 399658 | 91.0 | 201.4  | 171.4 | 231.4 |



# Quantitation Results Report (QT Reviewed)






# Quantitation Results Report (QT Reviewed)

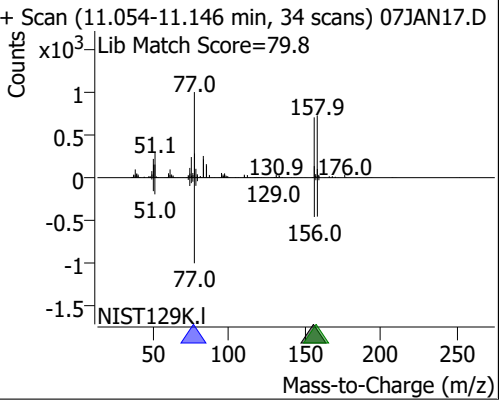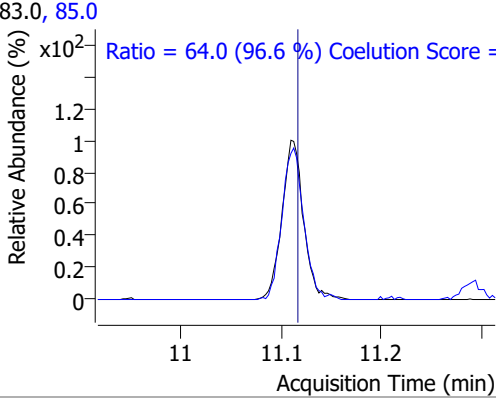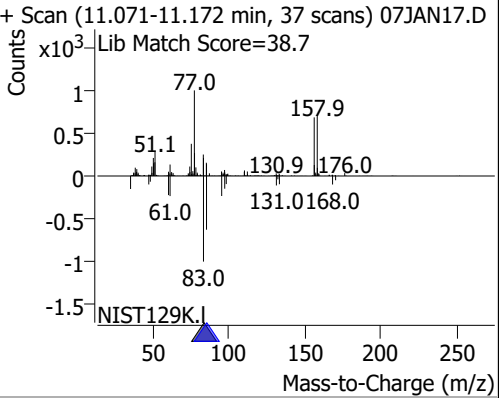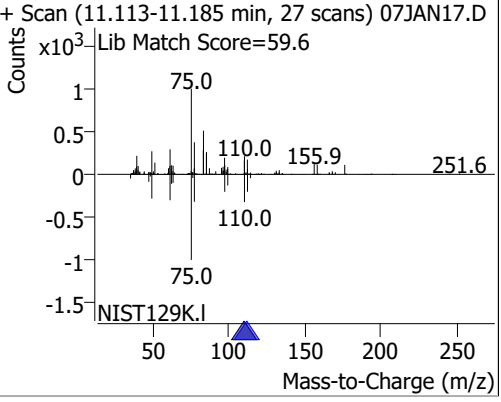

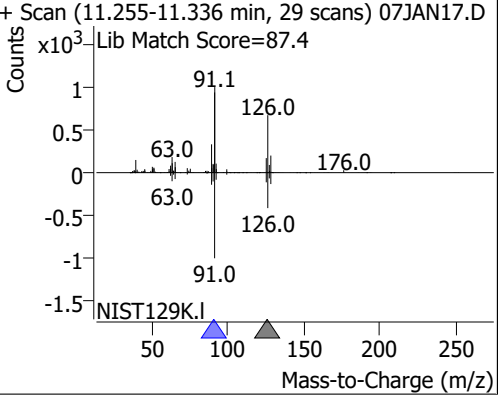
| Compound                                                                           | Conc.    | RT    | Dev(Min)                                                                             | Resp.  | QIon          | QRatio                                                                                | Lower         | Upper          |
|------------------------------------------------------------------------------------|----------|-------|--------------------------------------------------------------------------------------|--------|---------------|---------------------------------------------------------------------------------------|---------------|----------------|
| Bromobenzene                                                                       | 133.6149 | 11.09 | 0.00                                                                                 | 114173 | 77.0<br>158.0 | 146.4<br>98.5                                                                         | 115.7<br>66.5 | 175.7<br>126.5 |
|    |          |       |    |        |               |    |               |                |
| 1,1,2,2-Tetrachloroethane                                                          | 131.2329 | 11.11 | -0.01                                                                                | 64543  | 85.0          | 64.0                                                                                  | 36.2          | 96.2           |
|   |          |       |   |        |               |   |               |                |
| 1,2,3-Trichloropropane                                                             | 123.8246 | 11.14 | 0.00                                                                                 | 16295  | 112.0         | 65.0                                                                                  | 33.5          | 93.5           |
|  |          |       |  |        |               |  |               |                |
| 2-Chlorotoluene                                                                    | 131.3133 | 11.29 | 0.00                                                                                 | 111645 | 91.0          | 284.3                                                                                 | 252.3         | 312.3          |
|  |          |       |  |        |               |  |               |                |

# Quantitation Results Report (QT Reviewed)




| Compound        | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|-----------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 4-Chlorotoluene | 133.3048 | 11.40 | 0.00     | 369533 | 126.0 | 32.0   | 1.7   | 61.7  |



| Compound            | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,3-Dichlorobenzene | 131.3970 | 12.03 | 0.00     | 204772 | 148.0 | 64.4   | 33.6  | 93.6  |
|                     |          |       |          |        | 111.0 | 39.4   | 9.8   | 69.8  |






| Compound            | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,4-Dichlorobenzene | 129.8964 | 12.13 | 0.00     | 206411 | 148.0 | 63.6   | 33.1  | 93.1  |
|                     |          |       |          |        | 111.0 | 38.6   | 9.1   | 69.1  |



# Quantitation Results Report (QT Reviewed)


| Compound            | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,2-Dichlorobenzene | 125.9590 | 12.49 | 0.00     | 165895 | 148.0 | 64.8   | 33.9  | 93.9  |
|                     |          |       |          |        | 111.0 | 41.1   | 11.0  | 71.0  |

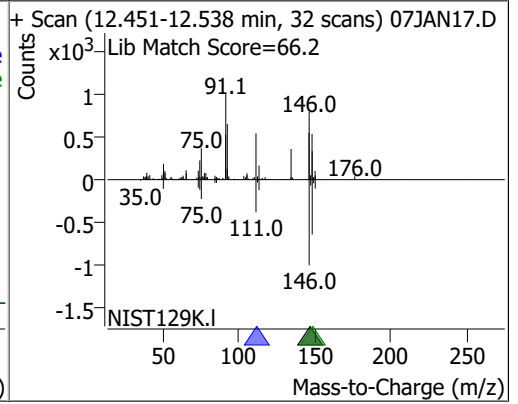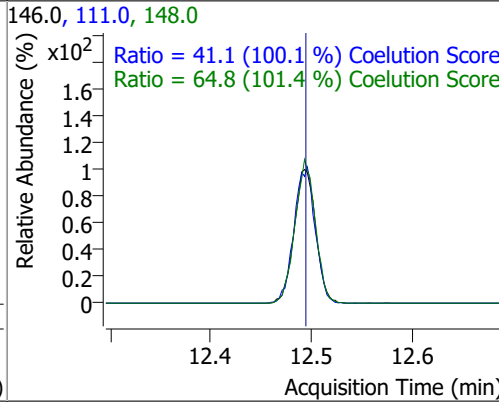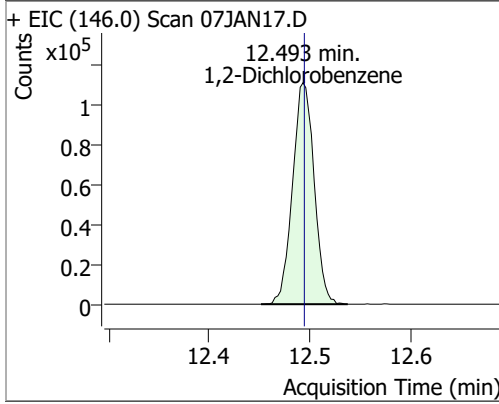



# Quantitation Results Report (QT Reviewed)

|                |                                     |                   |                       |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File      | 07JAN18.D                           | Operator          | MSC                   |
| Acq. Method    | 5975CACQF.M                         | Acq. Date-Time    | 1/7/2022 5:34:50 PM   |
| Sample Name    | B22010219-001FMSD                   | Instrument        | VOA5975C              |
| Vial           | 18                                  | Multiplier        | 1.00                  |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m  | Comment           |                       |
| Tune File      | BFB_Atune3.u                        | Tune Date         | 10/11/2021 4:02:00 PM |
| Batch Name     | VG010722_8260B.batch.bin            | Last Calib Update | 3/2/2022 10:41:44 AM  |
| Ref Library    | \\MASSHUNTER\Org\Library\NIST129K.l |                   |                       |

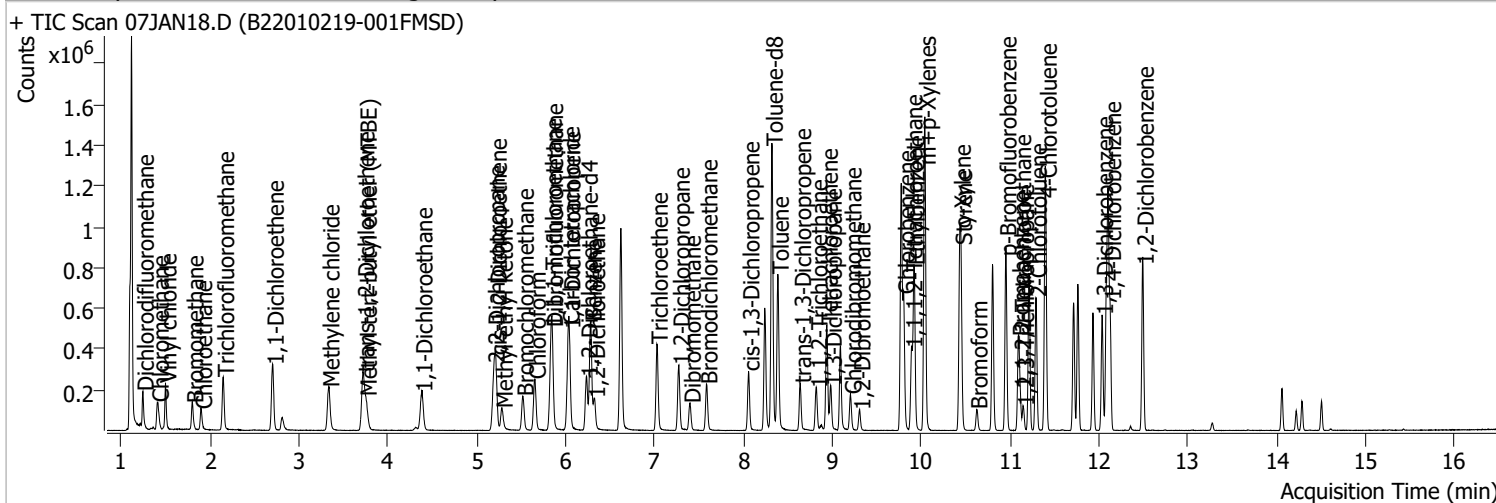









| Compound                           | RT                   | QIon  | Resp.  | Conc.              | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|--------------------|-------|----------|
| <b>Internal Standards</b>          |                      |       |        |                    |       |          |
| M Fluorobenzene                    | 6.621                | 96.0  | 847841 | 250.0000           | ng    | -0.003   |
| M Chlorobenzene-d5                 | 9.772                | 82.0  | 322063 | 250.0000           | ng    | 0.000    |
| M 1,4-Dichlorobenzene-d4           | 12.100               | 152.0 | 260394 | 250.0000           | ng    | 0.000    |
| <b>System Monitoring Compounds</b> |                      |       |        |                    |       |          |
| S Dibromofluoromethane             | 5.848                | 113.0 | 214547 | 268.6027           | ng    | 0.003    |
| Spiked Amount: 250.000             | Range: 80.0 - 119.0% |       |        | Recovery = 107.44% |       |          |
| S 1,2-Dichloroethane-d4            | 6.236                | 67.0  | 94029  | 272.5452           | ng    | 0.003    |
| Spiked Amount: 250.000             | Range: 81.0 - 118.0% |       |        | Recovery = 109.02% |       |          |
| S Toluene-d8                       | 8.319                | 98.0  | 857800 | 276.3920           | ng    | 0.000    |
| Spiked Amount: 250.000             | Range: 89.0 - 112.0% |       |        | Recovery = 110.56% |       |          |
| S p-Bromofluorobenzene             | 10.949               | 95.0  | 258687 | 271.1727           | ng    | -0.006   |
| Spiked Amount: 250.000             | Range: 85.0 - 114.0% |       |        | Recovery = 108.47% |       |          |
| <b>Target Compounds</b>            |                      |       |        |                    |       |          |
| T Dichlorodifluoromethane          | 1.244                | 85.0  | 122916 | 110.6317           | ng    | 99       |
| T Chloromethane                    | 1.411                | 50.0  | 158746 | 117.7180           | ng    | 100      |
| T Vinyl chloride                   | 1.498                | 62.0  | 151717 | 125.0334           | ng    | 98       |
| T Bromomethane                     | 1.802                | 96.0  | 65044  | 119.8794           | ng    | 96       |
| T Chloroethane                     | 1.899                | 64.0  | 73037  | 121.5844           | ng    | 98       |
| T Trichlorofluoromethane           | 2.148                | 101.0 | 181247 | 120.3412           | ng    | 99       |
| T 1,1-Dichloroethene               | 2.705                | 96.0  | 114899 | 134.5404           | ng    | 99       |
| T Methylene chloride               | 3.333                | 49.0  | 158297 | 125.7372           | ng    | 99       |
| T trans-1,2-Dichloroethene         | 3.723                | 96.0  | 120311 | 138.0852           | ng    | 99       |
| T Methyl tert-butyl ether (MTBE)   | 3.751                | 73.0  | 161012 | 142.9708           | ng    | 100      |
| T 1,1-Dichloroethane               | 4.379                | 63.0  | 226152 | 139.4457           | ng    | 99       |
| T 2,2-Dichloropropane              | 5.193                | 77.0  | 171641 | 141.2419           | ng    | 99       |
| T cis-1,2-Dichloroethene           | 5.212                | 96.0  | 118290 | 133.9099           | ng    | 99       |
| T Methyl ethyl ketone              | 5.282                | 43.0  | 145750 | 1218.1021          | ng    | 99       |
| T Bromochloromethane               | 5.519                | 128.0 | 46796  | 127.8755           | ng    | 97       |
| T Chloroform                       | 5.653                | 83.0  | 203762 | 126.2450           | ng    | 100      |

# Quantitation Results Report (QT Reviewed)

| Compound                    | RT     | QIon  | Resp.  | Conc.    | Units | Dev(Min) |
|-----------------------------|--------|-------|--------|----------|-------|----------|
| T 1,1,1-Trichloroethane     | 5.834  | 97.0  | 196145 | 129.6747 | ng    | 99       |
| T Carbon tetrachloride      | 6.029  | 117.0 | 185767 | 124.6502 | ng    | 97       |
| T 1,1-Dichloropropene       | 6.041  | 75.0  | 161545 | 125.6088 | ng    | 99       |
| T Benzene                   | 6.283  | 78.0  | 449224 | 133.0746 | ng    | 99       |
| T 1,2-Dichloroethane        | 6.319  | 62.0  | 116685 | 127.7729 | ng    | 96       |
| T Trichloroethene           | 7.025  | 95.0  | 129711 | 133.5436 | ng    | 99       |
| T 1,2-Dichloropropane       | 7.270  | 63.0  | 113897 | 133.3077 | ng    | 98       |
| T Dibromomethane            | 7.396  | 93.0  | 46728  | 129.4203 | ng    | 97       |
| T Bromodichloromethane      | 7.583  | 83.0  | 134905 | 135.3871 | ng    | 98       |
| T cis-1,3-Dichloropropene   | 8.057  | 75.0  | 143696 | 127.5477 | ng    | 98       |
| T Toluene                   | 8.386  | 92.0  | 289892 | 138.2772 | ng    | 98       |
| T trans-1,3-Dichloropropene | 8.637  | 75.0  | 108822 | 135.6987 | ng    | 98       |
| T 1,1,2-Trichloroethane     | 8.821  | 83.0  | 53613  | 128.3504 | ng    | 97       |
| T Tetrachloroethene         | 8.938  | 163.8 | 112970 | 132.0855 | ng    | 98       |
| T 1,3-Dichloropropane       | 8.983  | 76.0  | 109032 | 132.7040 | ng    | 98       |
| T Chlorodibromomethane      | 9.203  | 129.0 | 83383  | 127.7253 | ng    | 99       |
| T 1,2-Dibromoethane         | 9.303  | 107.0 | 60123  | 131.6380 | ng    | 99       |
| T Chlorobenzene             | 9.802  | 112.0 | 312027 | 135.9465 | ng    | 100      |
| T 1,1,1,2-Tetrachloroethane | 9.889  | 131.0 | 101872 | 126.9708 | ng    | 99       |
| T Ethylbenzene              | 9.917  | 91.0  | 539120 | 135.4342 | ng    | 99       |
| T m+p-Xylenes               | 10.039 | 106.0 | 410298 | 265.2312 | ng    | 97       |
| T o-Xylene                  | 10.433 | 106.0 | 191917 | 139.3598 | ng    | 98       |
| T Styrene                   | 10.447 | 104.0 | 313760 | 141.5106 | ng    | 99       |
| T Bromoform                 | 10.622 | 172.5 | 46577  | 139.7801 | ng    | 97       |
| T Bromobenzene              | 11.091 | 156.0 | 120119 | 142.5401 | ng    | 98       |
| T 1,1,2,2-Tetrachloroethane | 11.113 | 83.0  | 66475  | 137.0521 | ng    | 95       |
| T 1,2,3-Trichloropropane    | 11.147 | 110.0 | 17465  | 134.5721 | ng    | 99       |
| T 2-Chlorotoluene           | 11.289 | 126.0 | 118405 | 141.2126 | ng    | 100      |
| T 4-Chlorotoluene           | 11.400 | 91.0  | 388335 | 142.0473 | ng    | 100      |
| T 1,3-Dichlorobenzene       | 12.033 | 146.0 | 212018 | 137.9499 | ng    | 99       |
| T 1,4-Dichlorobenzene       | 12.123 | 146.0 | 215367 | 137.4287 | ng    | 99       |
| T 1,2-Dichlorobenzene       | 12.493 | 146.0 | 172710 | 132.9681 | ng    | 99       |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (\*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

# Quantitation Results Report (QT Reviewed)

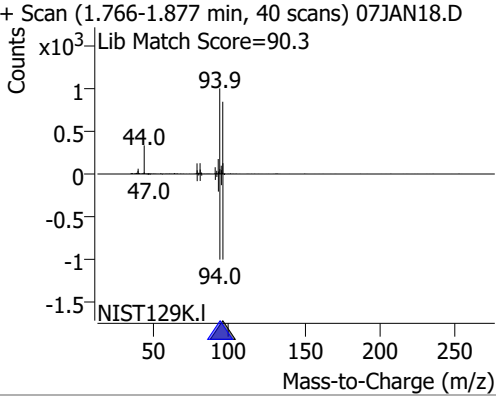
| Compound                                                                           | Conc.                                   | RT   | Dev(Min)                                                                              | Resp.  | QIon | QRatio                                       | Lower | Upper |
|------------------------------------------------------------------------------------|-----------------------------------------|------|---------------------------------------------------------------------------------------|--------|------|----------------------------------------------|-------|-------|
| Dichlorodifluoromethane                                                            | 110.6317                                | 1.24 | 0.00                                                                                  | 122916 | 87.0 | 32.7                                         | 2.3   | 62.3  |
| + EIC (85.0) Scan 07JAN18.D                                                        |                                         |      | 85.0, 87.0                                                                            |        |      | + Scan (1.213-1.336 min, 45 scans) 07JAN18.D |       |       |
|    | Ratio = 32.7 (101.4 %) Coelution Score  |      |    |        |      |                                              |       |       |
| Chloromethane                                                                      | 117.7180                                | 1.41 | 0.00                                                                                  | 158746 | 52.0 | 32.3                                         | 2.1   | 62.1  |
| + EIC (50.0) Scan 07JAN18.D                                                        |                                         |      | 50.0, 52.0                                                                            |        |      | + Scan (1.375-1.531 min, 57 scans) 07JAN18.D |       |       |
|   | Ratio = 32.3 (100.5 %) Coelution Score  |      |   |        |      |                                              |       |       |
| Vinyl chloride                                                                     | 125.0334                                | 1.50 | 0.00                                                                                  | 151717 | 64.0 | 31.2                                         | 0.0   | 59.9  |
| + EIC (62.0) Scan 07JAN18.D                                                        |                                         |      | 62.0, 64.0                                                                            |        |      | + Scan (1.470-1.579 min, 40 scans) 07JAN18.D |       |       |
|  | Ratio = 31.2 (104.2 %) Coelution Score  |      |  |        |      |                                              |       |       |
| Bromomethane                                                                       | 119.8794                                | 1.80 | 0.00                                                                                  | 65044  | 94.0 | 108.7                                        | 74.6  | 134.6 |
| + EIC (96.0) Scan 07JAN18.D                                                        |                                         |      | 96.0, 94.0                                                                            |        |      | + Scan (1.766-1.877 min, 40 scans) 07JAN18.D |       |       |
|  | Ratio = 108.7 (103.8 %) Coelution Score |      |  |        |      |                                              |       |       |

# Quantitation Results Report (QT Reviewed)


| Compound     | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|----------|------|----------|-------|------|--------|-------|-------|
| Chloroethane | 121.5844 | 1.90 | 0.01     | 73037 | 66.0 | 31.4   | 0.1   | 60.1  |

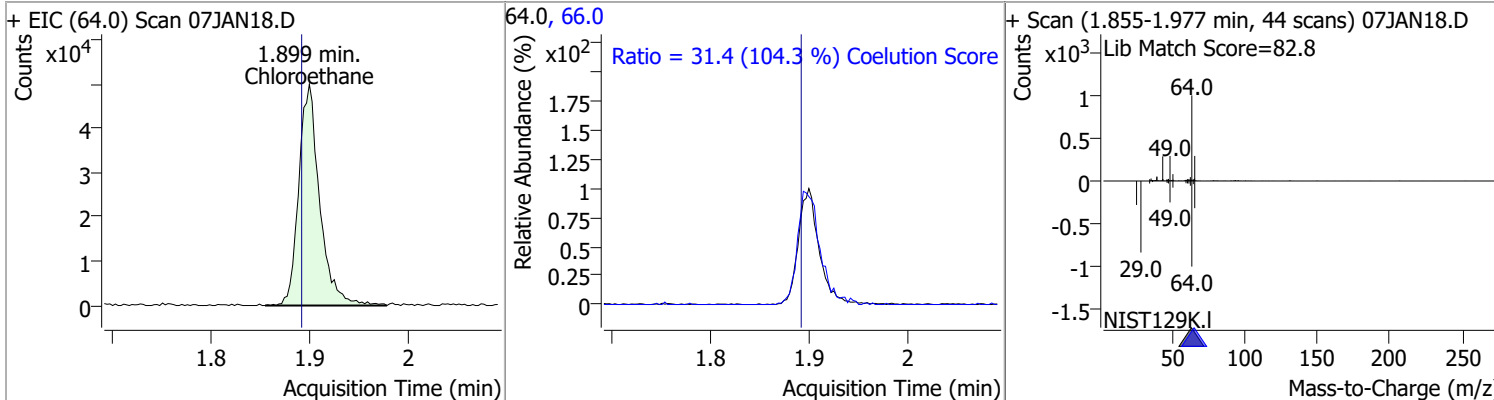


| Compound               | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|------------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Trichlorofluoromethane | 120.3412 | 2.15 | 0.01     | 181247 | 103.0 | 63.8   | 34.2  | 94.2  |

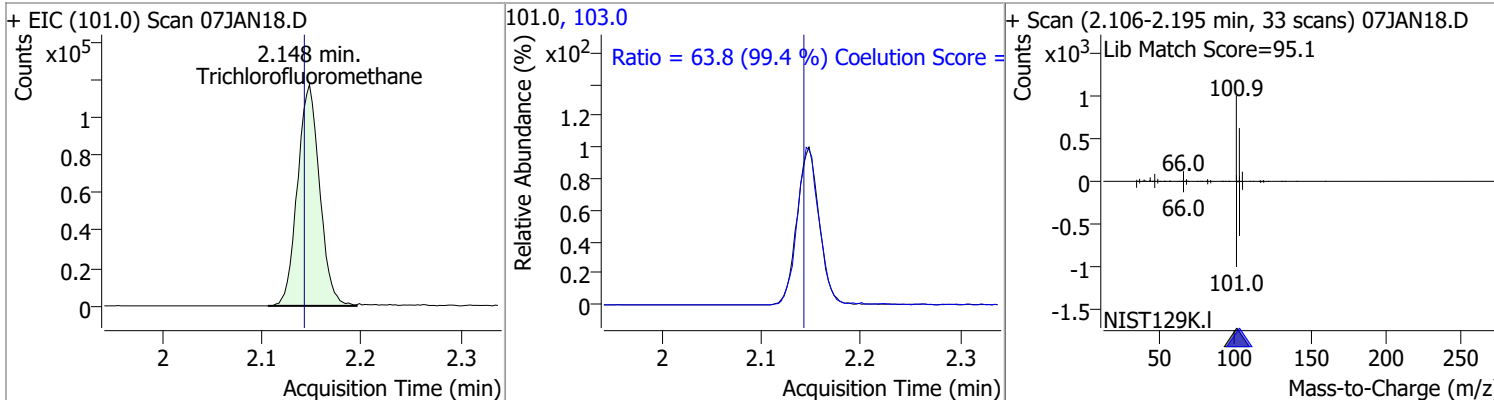

| Compound           | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1-Dichloroethene | 134.5404 | 2.71 | 0.01     | 114899 | 61.0 | 182.0  | 150.3 | 210.3 |
|                    |          |      |          |        | 63.0 | 58.0   | 26.7  | 86.7  |

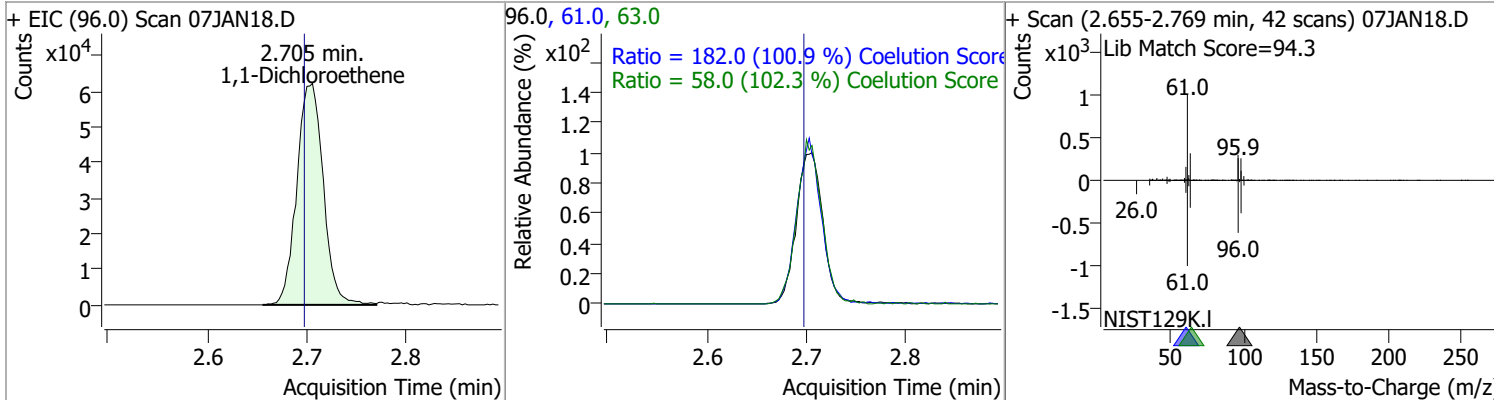


| Compound           | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| Methylene chloride | 125.7372 | 3.33 | 0.00     | 158297 | 84.0 | 66.4   | 36.9  | 96.9  |
|                    |          |      |          |        | 86.0 | 43.0   | 14.3  | 74.3  |

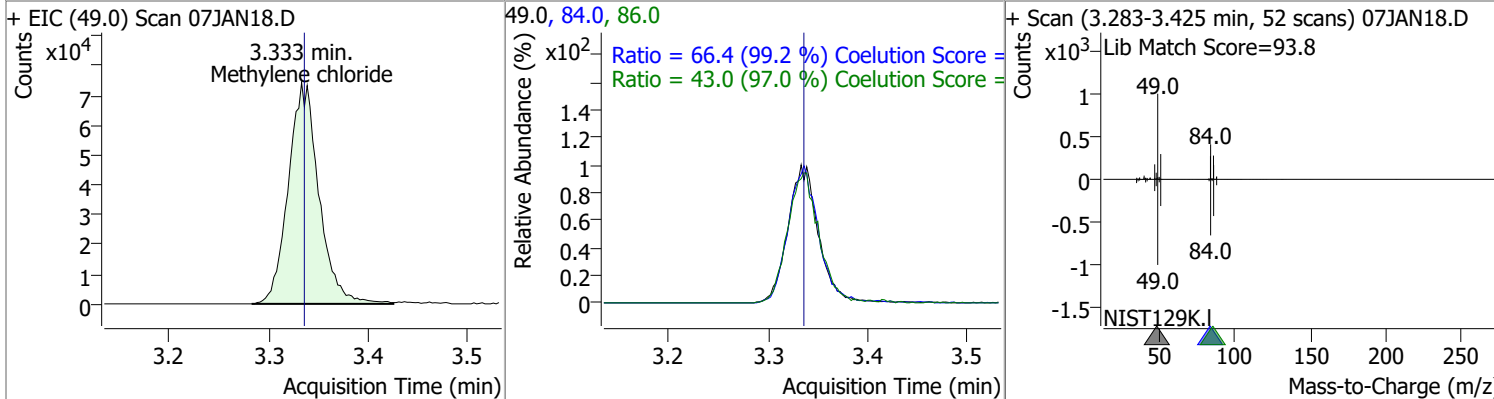


# Quantitation Results Report (QT Reviewed)


| Compound                 | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------------|----------|------|----------|--------|------|--------|-------|-------|
| trans-1,2-Dichloroethene | 138.0852 | 3.72 | 0.01     | 120311 | 61.0 | 152.1  | 123.9 | 183.9 |
|                          |          |      |          |        | 98.0 | 64.4   | 35.7  | 95.7  |

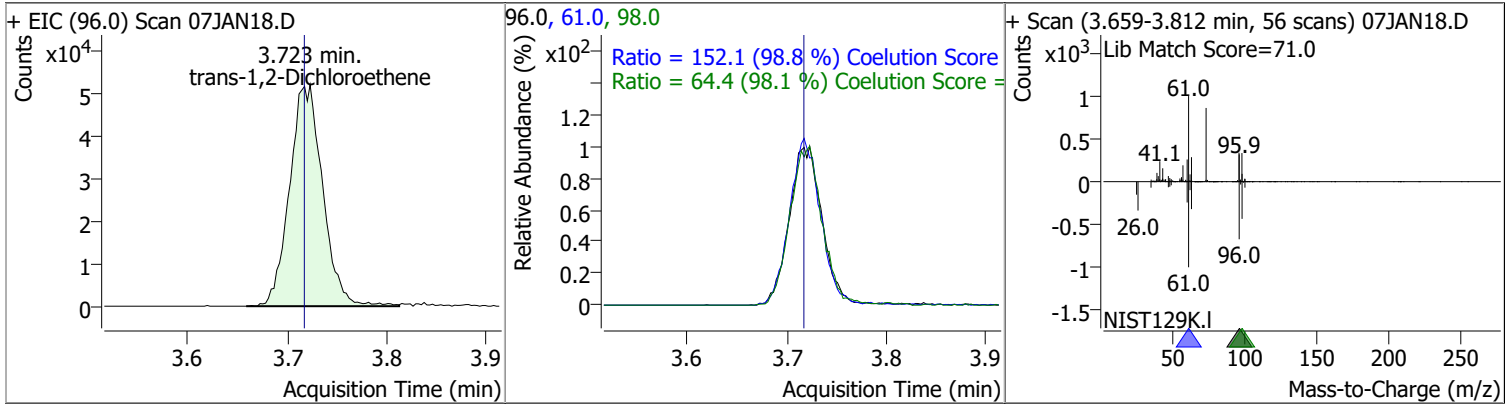

| Compound                       | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------------------|----------|------|----------|--------|------|--------|-------|-------|
| Methyl tert-butyl ether (MTBE) | 142.9708 | 3.75 | 0.00     | 161012 | 57.0 | 24.4   | 0.0   | 54.6  |

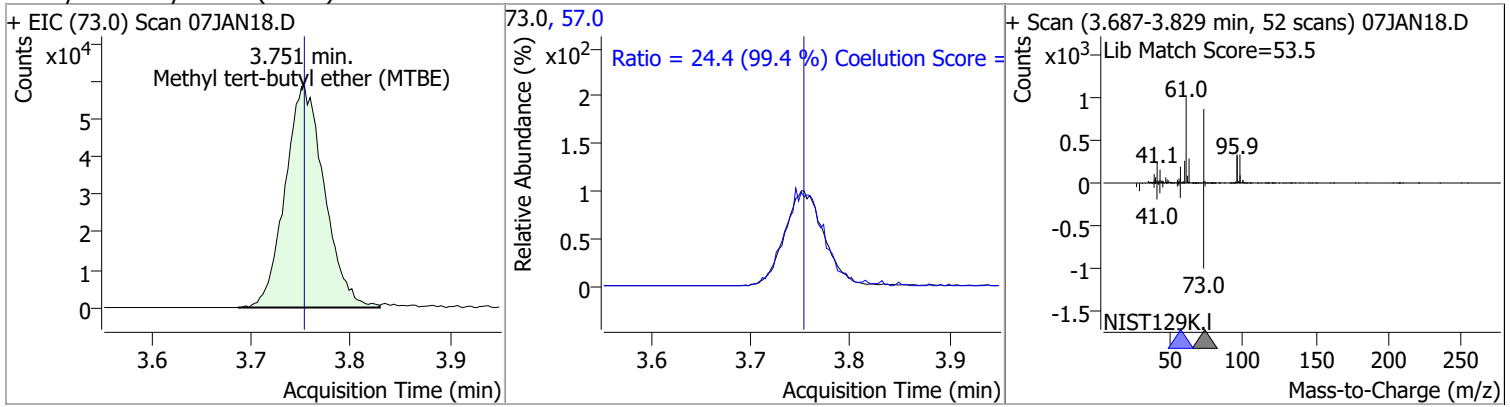


| Compound           | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1-Dichloroethane | 139.4457 | 4.38 | 0.00     | 226152 | 65.0 | 32.2   | 2.1   | 62.1  |
|                    |          |      |          |        | 83.0 | 12.7   | 0.0   | 43.7  |

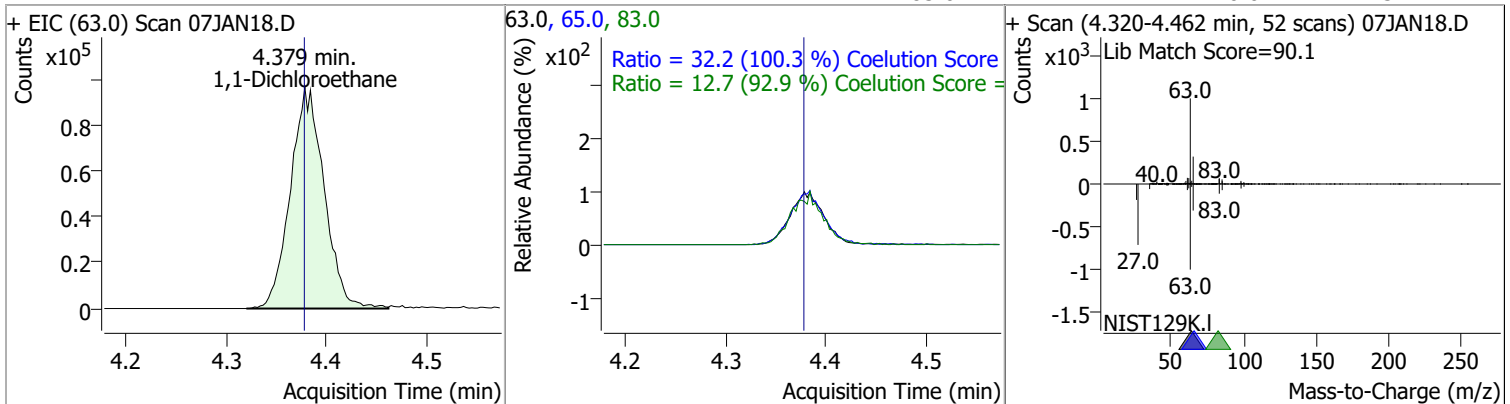


# Quantitation Results Report (QT Reviewed)


| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 2,2-Dichloropropane | 141.2419 | 5.19 | 0.00     | 171641 | 41.0 | 65.5   | 36.5  | 96.5  |
|                     |          |      |          |        | 97.0 | 22.4   | 0.0   | 53.2  |

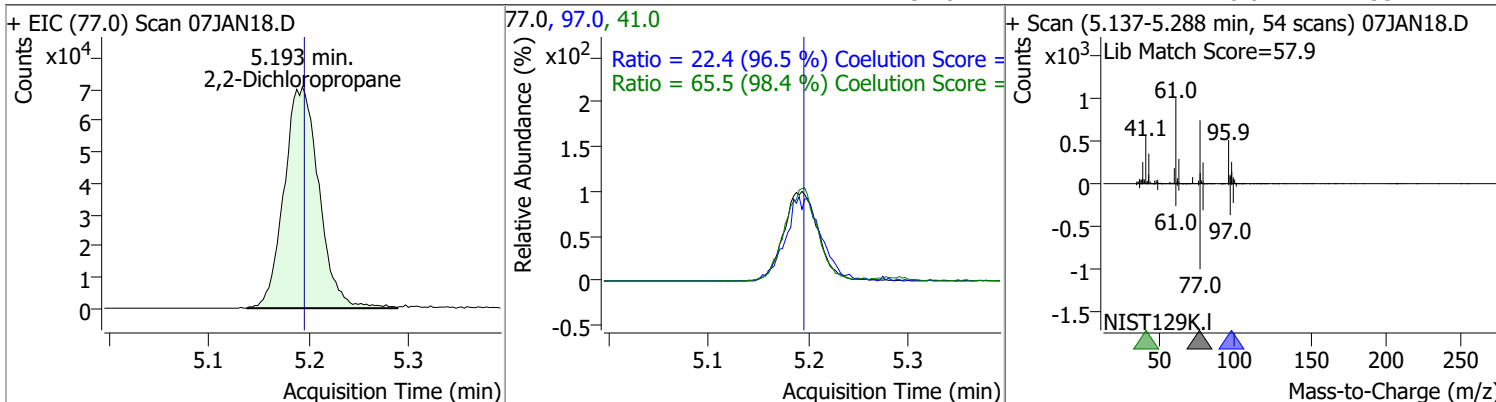


| Compound               | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,2-Dichloroethene | 133.9099 | 5.21 | 0.00     | 118290 | 61.0 | 169.7  | 137.2 | 197.2 |
|                        |          |      |          |        | 98.0 | 67.4   | 37.3  | 97.3  |

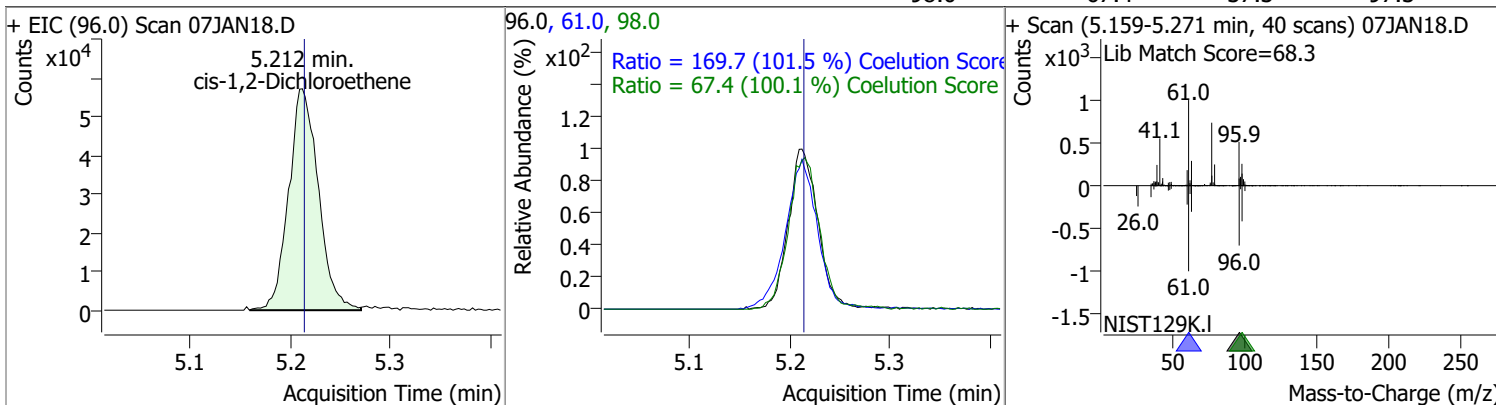

| Compound            | Conc.     | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|-----------|------|----------|--------|------|--------|-------|-------|
| Methyl ethyl ketone | 1218.1021 | 5.28 | 0.00     | 145750 | 72.0 | 22.0   | 0.0   | 51.3  |

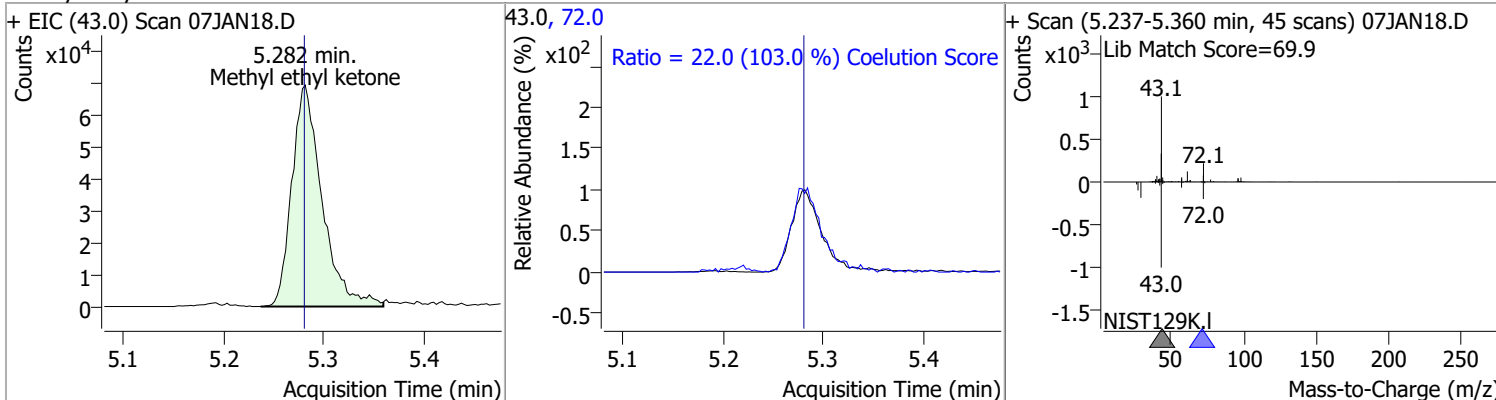


| Compound           | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|-------|------|--------|-------|-------|
| Bromochloromethane | 127.8755 | 5.52 | 0.00     | 46796 | 49.0 | 187.2  | 152.9 | 212.9 |

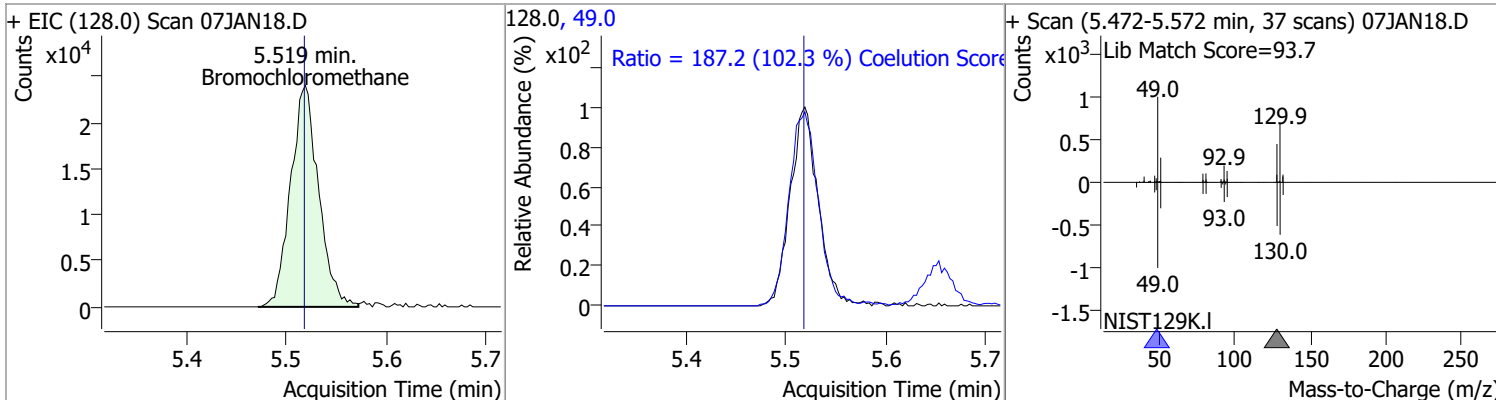


# Quantitation Results Report (QT Reviewed)


| Compound   | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|------|--------|-------|-------|
| Chloroform | 126.2450 | 5.65 | 0.00     | 203762 | 85.0 | 66.1   | 36.0  | 96.0  |




| Compound              | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1,1-Trichloroethane | 129.6747 | 5.83 | 0.00     | 196145 | 99.0 | 64.1   | 34.7  | 94.7  |
|                       |          |      |          |        | 61.0 | 49.3   | 18.1  | 78.1  |



| Compound             | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Dibromofluoromethane | 268.6027 | 5.85 | 0.00     | 214547 | 191.5 | 22.0   | 0.0   | 53.1  |




| Compound             | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Carbon tetrachloride | 124.6502 | 6.03 | 0.01     | 185767 | 119.0 | 99.6   | 67.2  | 127.2 |
|                      |          |      |          |        | 121.0 | 32.3   | 0.1   | 60.1  |

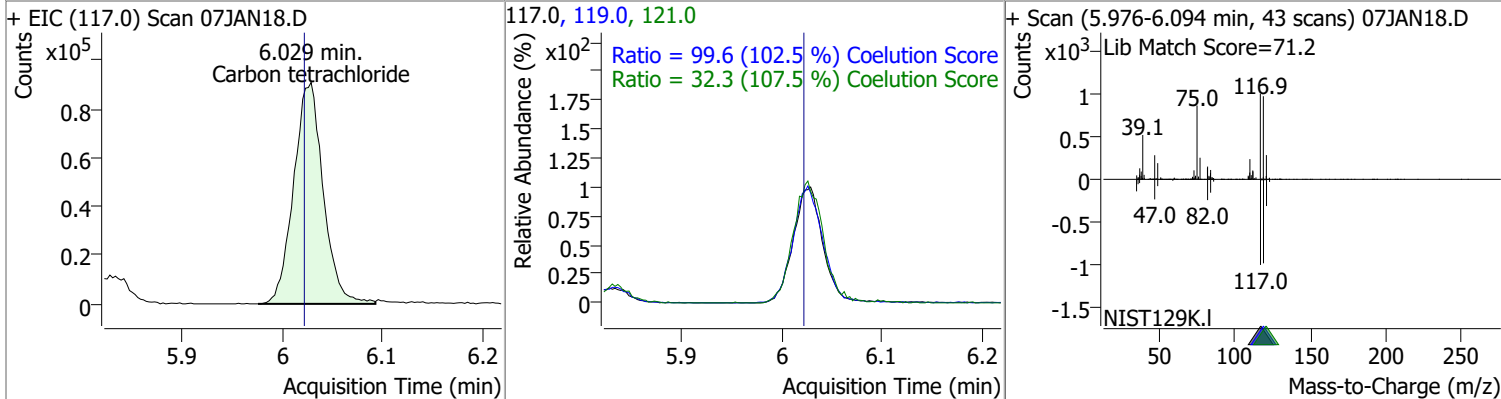


# Quantitation Results Report (QT Reviewed)


| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|-------|--------|-------|-------|
| 1,1-Dichloropropene | 125.6088 | 6.04 | 0.00     | 161545 | 110.0 | 36.8   | 5.9   | 65.9  |
|                     |          |      |          |        | 77.0  | 29.9   | 0.1   | 60.1  |

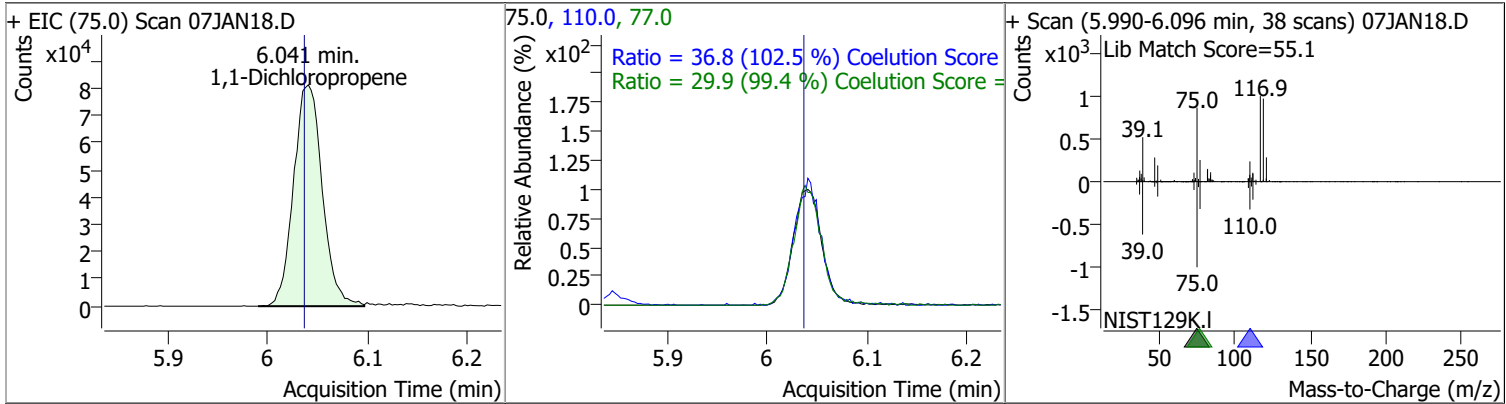


| Compound              | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 272.5452 | 6.24 | 0.00     | 94029 | 65.0 | 196.7  | 166.5 | 226.5 |

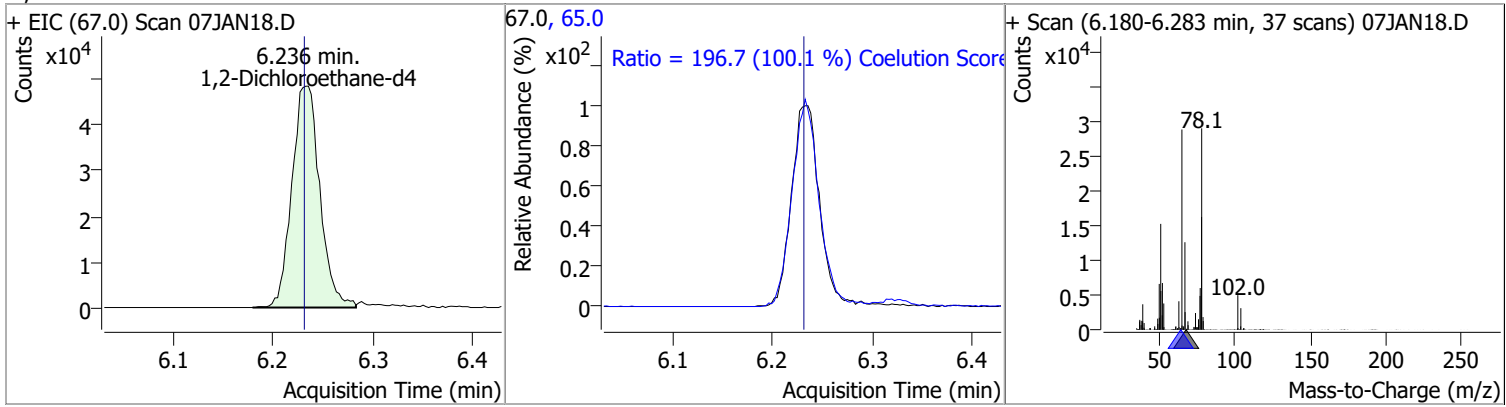

| Compound | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|----------|----------|------|----------|--------|------|--------|-------|-------|
| Benzene  | 133.0746 | 6.28 | 0.01     | 449224 | 77.0 | 24.1   | 0.0   | 53.5  |

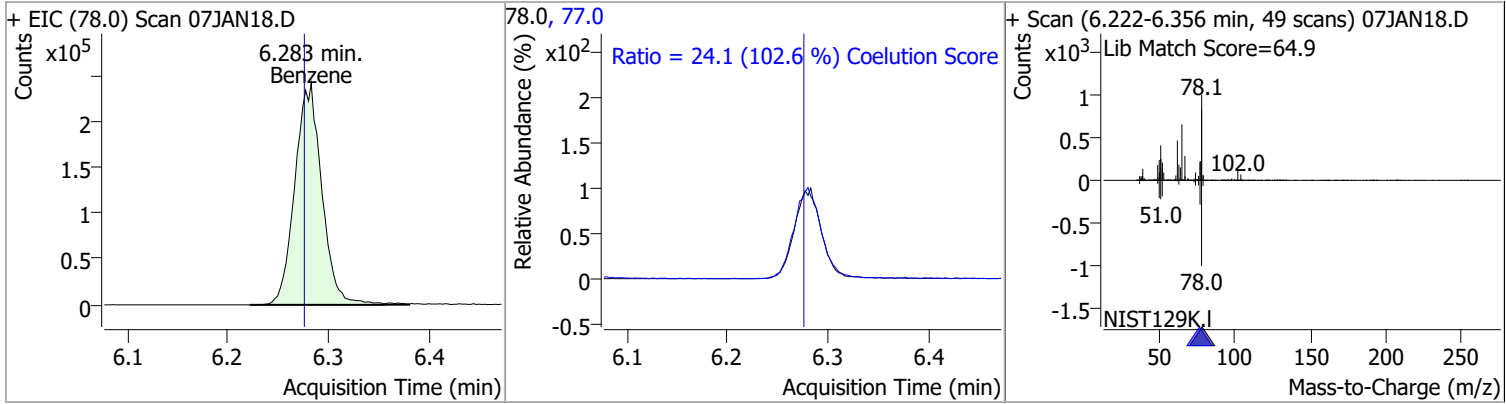


| Compound           | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloroethane | 127.7729 | 6.32 | 0.00     | 116685 | 64.0 | 32.3   | 0.0   | 59.9  |
|                    |          |      |          |        | 98.0 | 7.8    | 0.0   | 37.6  |

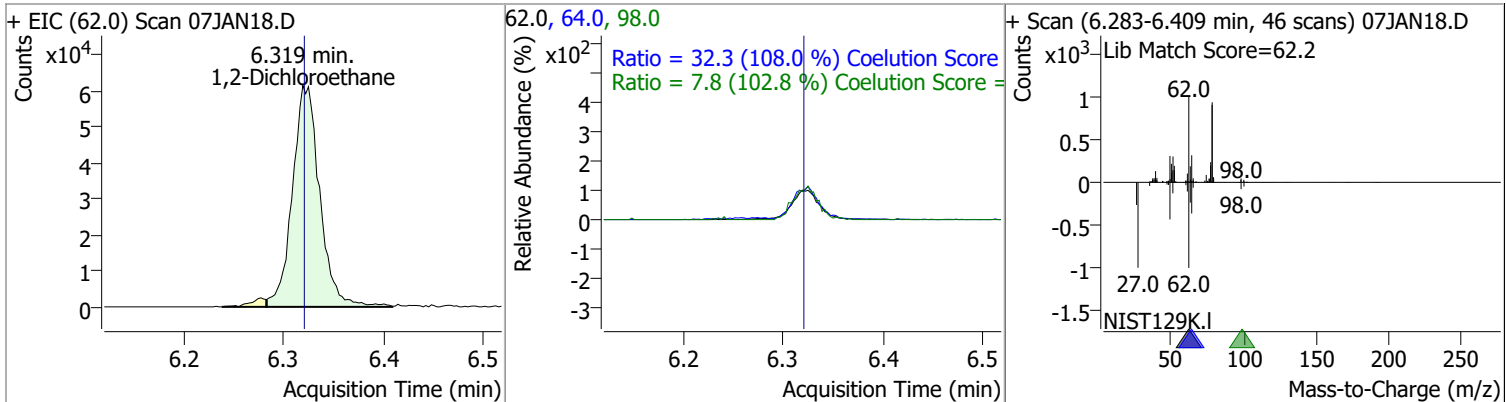




# Quantitation Results Report (QT Reviewed)


| Compound        | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|-----------------|----------|------|----------|--------|-------|--------|-------|-------|
| Trichloroethene | 133.5436 | 7.02 | -0.01    | 129711 | 130.0 | 102.3  | 71.5  | 131.5 |
|                 |          |      |          |        | 97.0  | 63.7   | 34.1  | 94.1  |

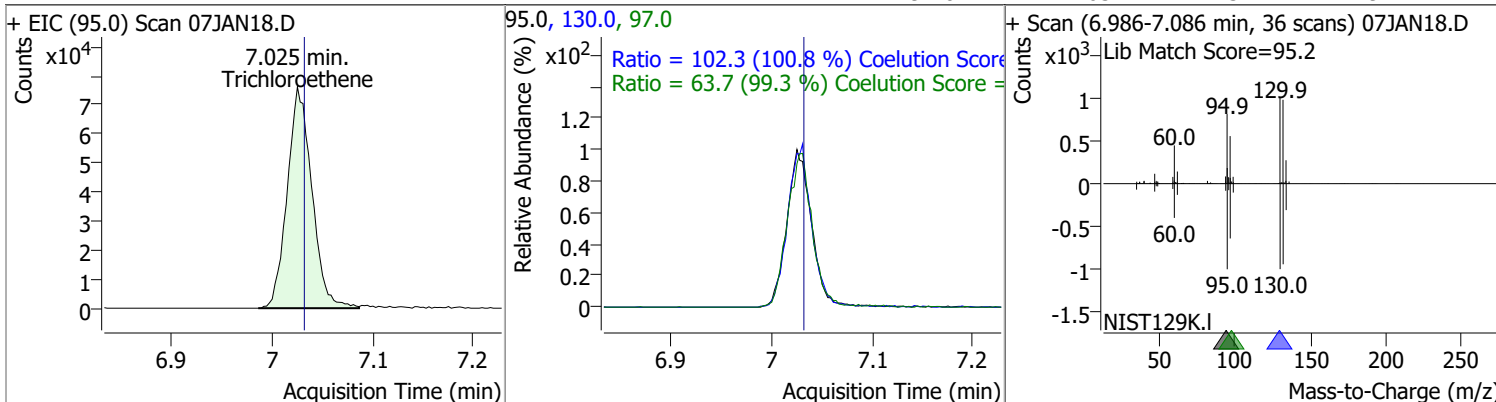

| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloropropane | 133.3077 | 7.27 | 0.00     | 113897 | 76.0 | 37.2   | 8.2   | 68.2  |

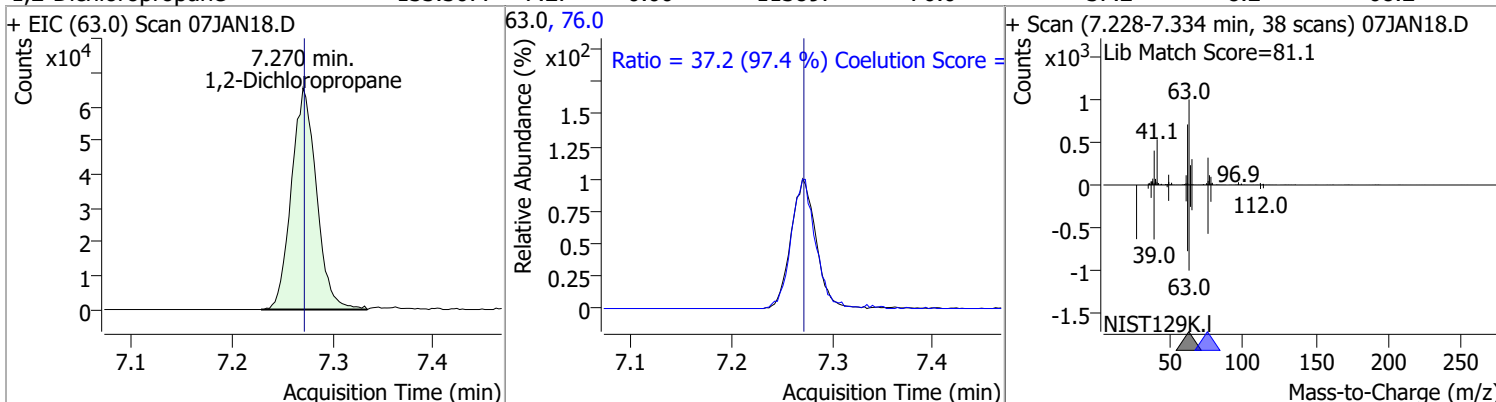


| Compound       | Conc.    | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|----------------|----------|------|----------|-------|-------|--------|-------|-------|
| Dibromomethane | 129.4203 | 7.40 | 0.00     | 46728 | 173.5 | 109.6  | 83.7  | 143.7 |
|                |          |      |          |       | 95.0  | 83.7   | 52.2  | 112.2 |

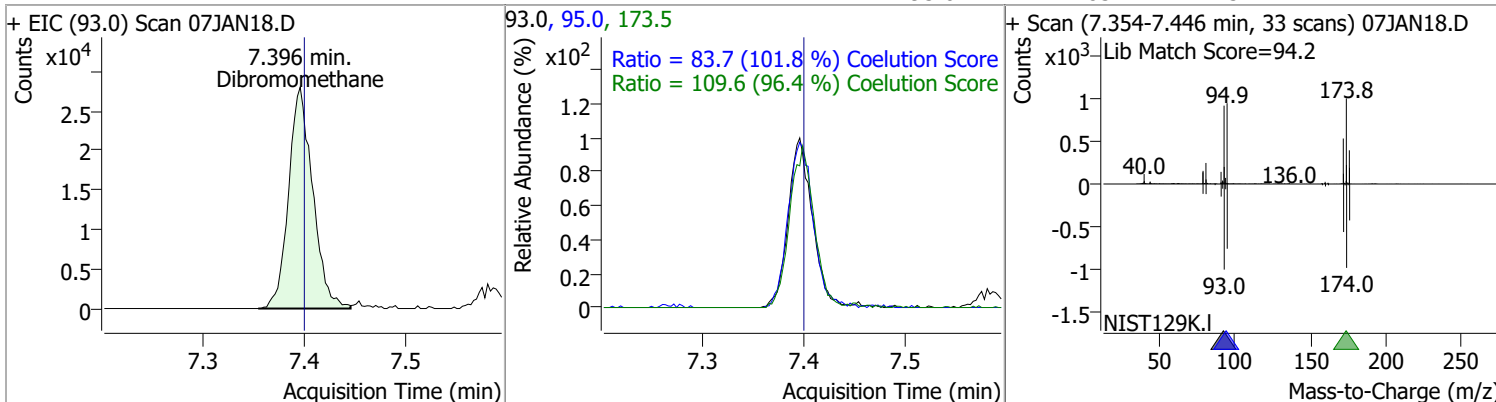


# Quantitation Results Report (QT Reviewed)


| Compound             | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Bromodichloromethane | 135.3871 | 7.58 | 0.00     | 134905 | 85.0  | 62.4   | 34.5  | 94.5  |
|                      |          |      |          |        | 127.0 | 9.1    | 0.0   | 39.6  |












| Compound                | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|-------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,3-Dichloropropene | 127.5477 | 8.06 | 0.00     | 143696 | 39.0 | 51.6   | 23.3  | 83.3  |
|                         |          |      |          |        | 77.0 | 31.2   | 1.0   | 61.0  |



| Compound   | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 276.3920 | 8.32 | 0.00     | 857800 | 100.0 | 63.8   | 34.4  | 94.4  |
|            |          |      |          |        | 99.0  | 9.7    | 0.0   | 39.6  |




# Quantitation Results Report (QT Reviewed)

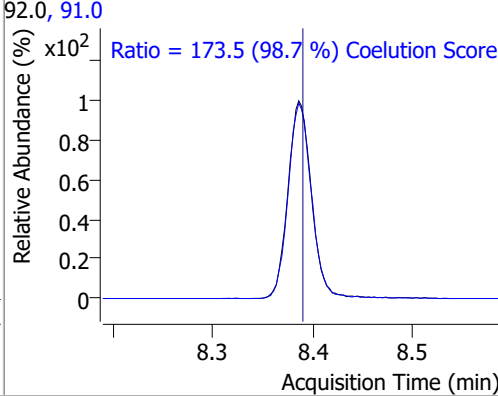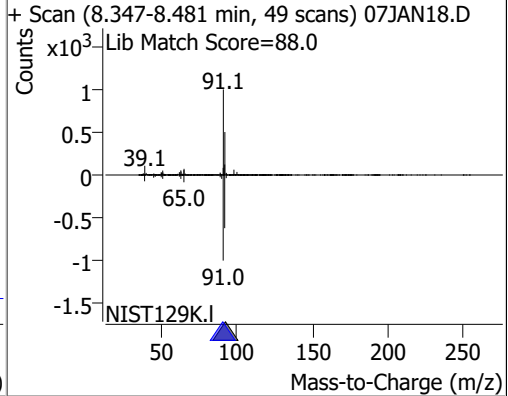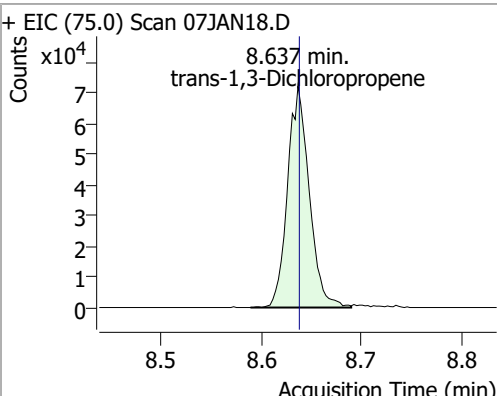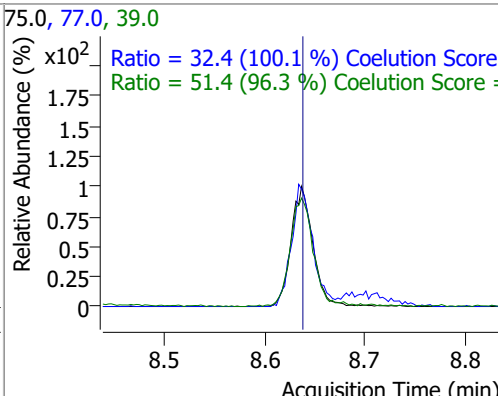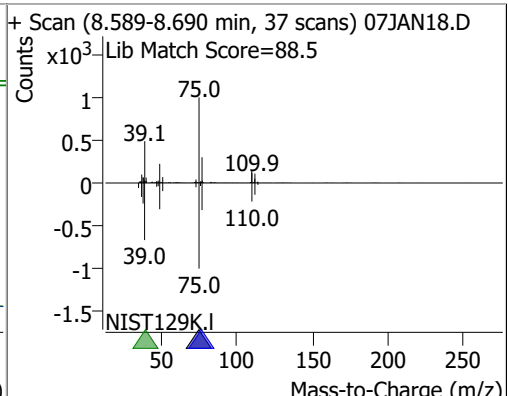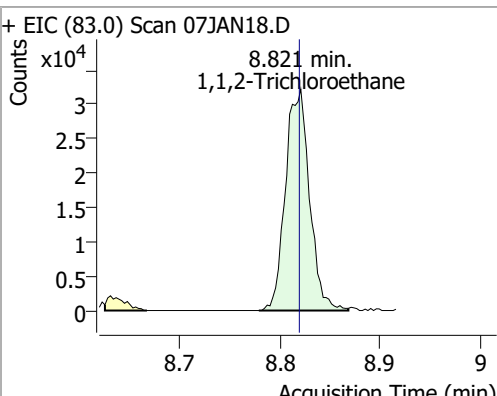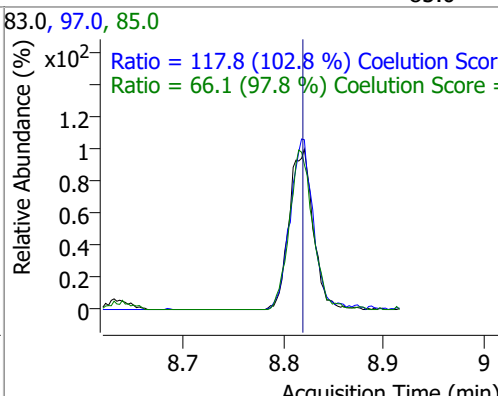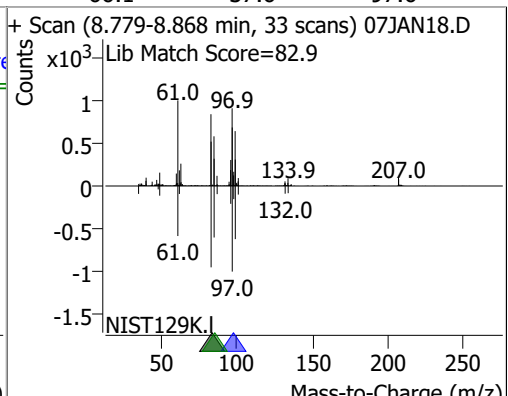
| Compound                                                                                                          | Conc.    | RT   | Dev(Min)                                                                                                 | Resp.  | QIon         | QRatio                                                                                                                                                        | Lower        | Upper         |
|-------------------------------------------------------------------------------------------------------------------|----------|------|----------------------------------------------------------------------------------------------------------|--------|--------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------|--------------|---------------|
| Toluene                                                                                                           | 138.2772 | 8.39 | 0.00                                                                                                     | 289892 | 91.0         | 173.5                                                                                                                                                         | 145.8        | 205.8         |
| + EIC (92.0) Scan 07JAN18.D<br>   |          |      | 92.0, 91.0<br>         |        |              | + Scan (8.347-8.481 min, 49 scans) 07JAN18.D<br>Lib Match Score=88.0<br>   |              |               |
|                                                                                                                   |          |      |                                                                                                          |        |              | Ratio = 173.5 (98.7 %) Coelution Score                                                                                                                        |              |               |
| trans-1,3-Dichloropropene                                                                                         | 135.6987 | 8.64 | 0.00                                                                                                     | 108822 | 39.0<br>77.0 | 51.4<br>32.4                                                                                                                                                  | 23.4<br>2.4  | 83.4<br>62.4  |
| + EIC (75.0) Scan 07JAN18.D<br>  |          |      | 75.0, 77.0, 39.0<br>  |        |              | + Scan (8.589-8.690 min, 37 scans) 07JAN18.D<br>Lib Match Score=88.5<br>  |              |               |
|                                                                                                                   |          |      |                                                                                                          |        |              | Ratio = 32.4 (100.1 %) Coelution Score                                                                                                                        |              |               |
|                                                                                                                   |          |      |                                                                                                          |        |              | Ratio = 51.4 (96.3 %) Coelution Score                                                                                                                         |              |               |
| 1,1,2-Trichloroethane                                                                                             | 128.3504 | 8.82 | 0.00                                                                                                     | 53613  | 97.0<br>85.0 | 117.8<br>66.1                                                                                                                                                 | 84.6<br>37.6 | 144.6<br>97.6 |
| + EIC (83.0) Scan 07JAN18.D<br> |          |      | 83.0, 97.0, 85.0<br> |        |              | + Scan (8.779-8.868 min, 33 scans) 07JAN18.D<br>Lib Match Score=82.9<br> |              |               |
|                                                                                                                   |          |      |                                                                                                          |        |              | Ratio = 117.8 (102.8 %) Coelution Score                                                                                                                       |              |               |
|                                                                                                                   |          |      |                                                                                                          |        |              | Ratio = 66.1 (97.8 %) Coelution Score                                                                                                                         |              |               |

# Quantitation Results Report (QT Reviewed)


| Compound          | Conc.    | RT   | Dev(Min) | Resp.  | QIon           | QRatio        | Lower        | Upper          |
|-------------------|----------|------|----------|--------|----------------|---------------|--------------|----------------|
| Tetrachloroethene | 132.0855 | 8.94 | 0.00     | 112970 | 165.8<br>129.0 | 124.7<br>90.5 | 98.6<br>61.5 | 158.6<br>121.5 |




| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,3-Dichloropropane | 132.7040 | 8.98 | 0.00     | 109032 | 78.0 | 31.6   | 2.9   | 62.9  |















| Compound             | Conc.    | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|----------------------|----------|------|----------|-------|-------|--------|-------|-------|
| Chlorodibromomethane | 127.7253 | 9.20 | 0.00     | 83383 | 127.0 | 79.2   | 48.0  | 108.0 |







| Compound          | Conc.    | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|-------------------|----------|------|----------|-------|-------|--------|-------|-------|
| 1,2-Dibromoethane | 131.6380 | 9.30 | 0.00     | 60123 | 109.0 | 93.8   | 64.5  | 124.5 |



# Quantitation Results Report (QT Reviewed)

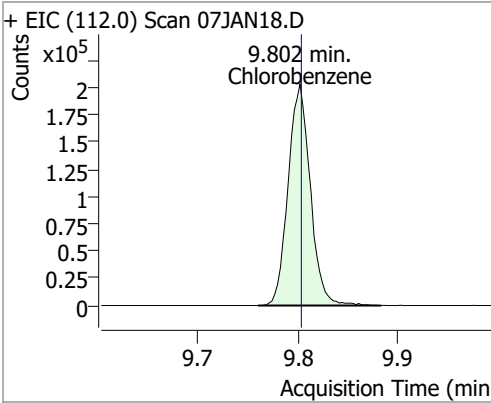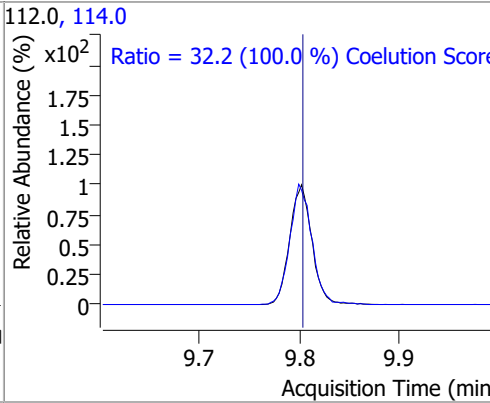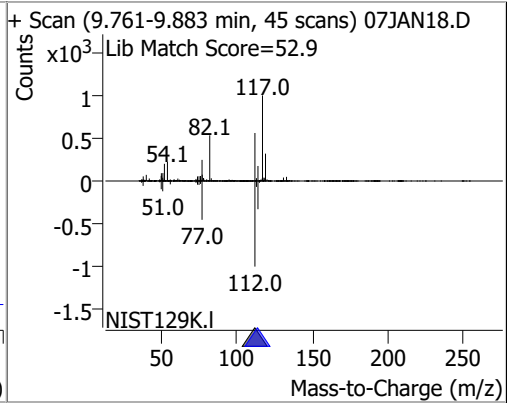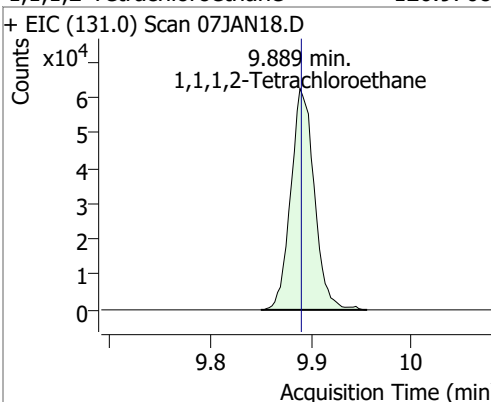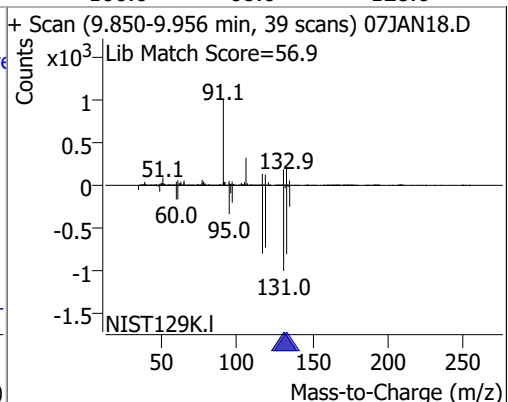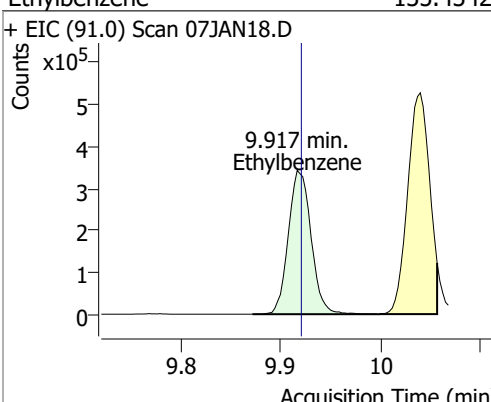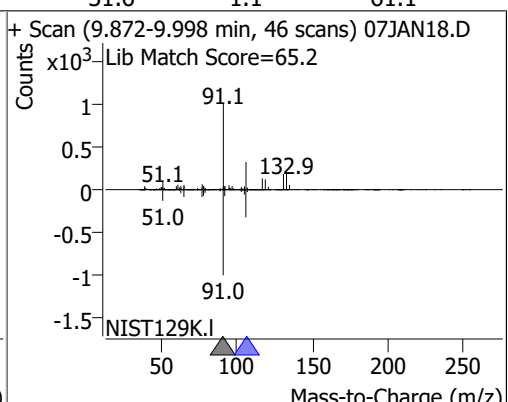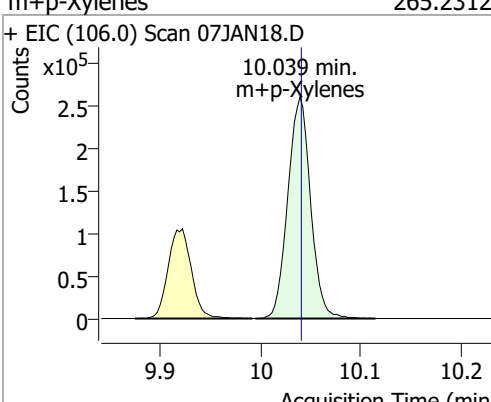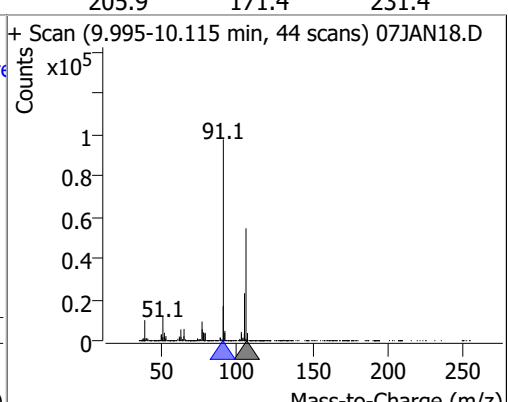
| Compound                                                                                                           | Conc.    | RT    | Dev(Min)                                                                                            | Resp.  | QIon  | QRatio                                                                                                                                                        | Lower | Upper |
|--------------------------------------------------------------------------------------------------------------------|----------|-------|-----------------------------------------------------------------------------------------------------|--------|-------|---------------------------------------------------------------------------------------------------------------------------------------------------------------|-------|-------|
| Chlorobenzene                                                                                                      | 135.9465 | 9.80  | 0.00                                                                                                | 312027 | 114.0 | 32.2                                                                                                                                                          | 2.1   | 62.1  |
| + EIC (112.0) Scan 07JAN18.D<br>   |          |       | 112.0, 114.0<br>  |        |       | + Scan (9.761-9.883 min, 45 scans) 07JAN18.D<br>Lib Match Score=52.9<br>   |       |       |
| 1,1,1,2-Tetrachloroethane                                                                                          | 126.9708 | 9.89  | 0.00                                                                                                | 101872 | 133.0 | 100.0                                                                                                                                                         | 68.6  | 128.6 |
| + EIC (131.0) Scan 07JAN18.D<br>  |          |       | 131.0, 133.0<br> |        |       | + Scan (9.850-9.956 min, 39 scans) 07JAN18.D<br>Lib Match Score=56.9<br>  |       |       |
| Ethylbenzene                                                                                                       | 135.4342 | 9.92  | 0.00                                                                                                | 539120 | 106.0 | 31.6                                                                                                                                                          | 1.1   | 61.1  |
| + EIC (91.0) Scan 07JAN18.D<br>  |          |       | 91.0, 106.0<br> |        |       | + Scan (9.872-9.998 min, 46 scans) 07JAN18.D<br>Lib Match Score=65.2<br> |       |       |
| m+p-Xylenes                                                                                                        | 265.2312 | 10.04 | 0.00                                                                                                | 410298 | 91.0  | 205.9                                                                                                                                                         | 171.4 | 231.4 |
| + EIC (106.0) Scan 07JAN18.D<br> |          |       | 106.0, 91.0<br> |        |       | + Scan (9.995-10.115 min, 44 scans) 07JAN18.D<br>                        |       |       |

# Quantitation Results Report (QT Reviewed)




# Quantitation Results Report (QT Reviewed)


| Compound     | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|--------------|----------|-------|----------|--------|-------|--------|-------|-------|
| Bromobenzene | 142.5401 | 11.09 | 0.00     | 120119 | 77.0  | 141.7  | 115.7 | 175.7 |
|              |          |       |          |        | 158.0 | 96.0   | 66.5  | 126.5 |

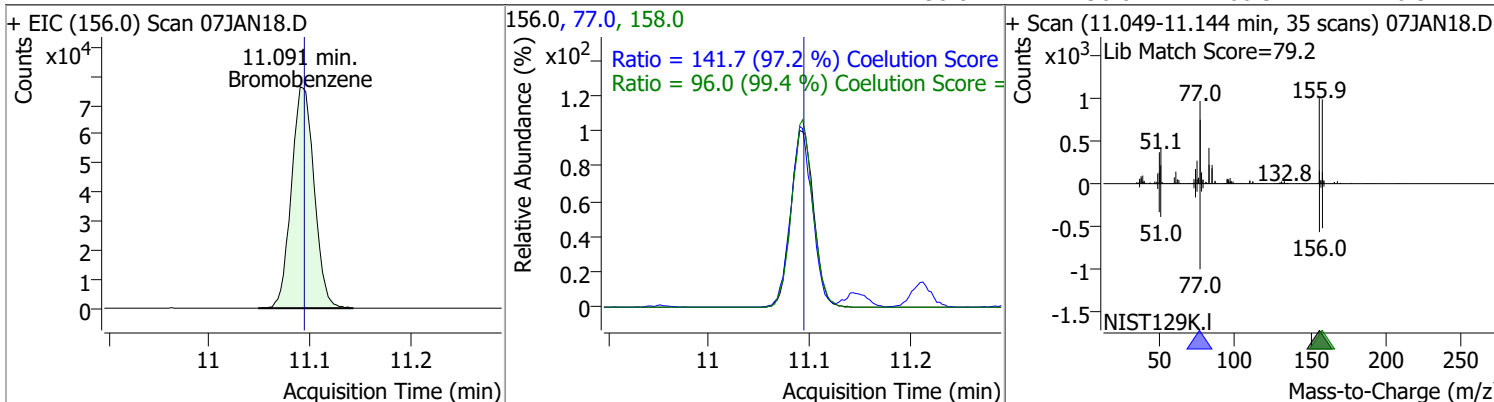


| Compound                  | Conc.    | RT    | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|----------|-------|----------|-------|------|--------|-------|-------|
| 1,1,2,2-Tetrachloroethane | 137.0521 | 11.11 | 0.00     | 66475 | 85.0 | 62.6   | 36.2  | 96.2  |

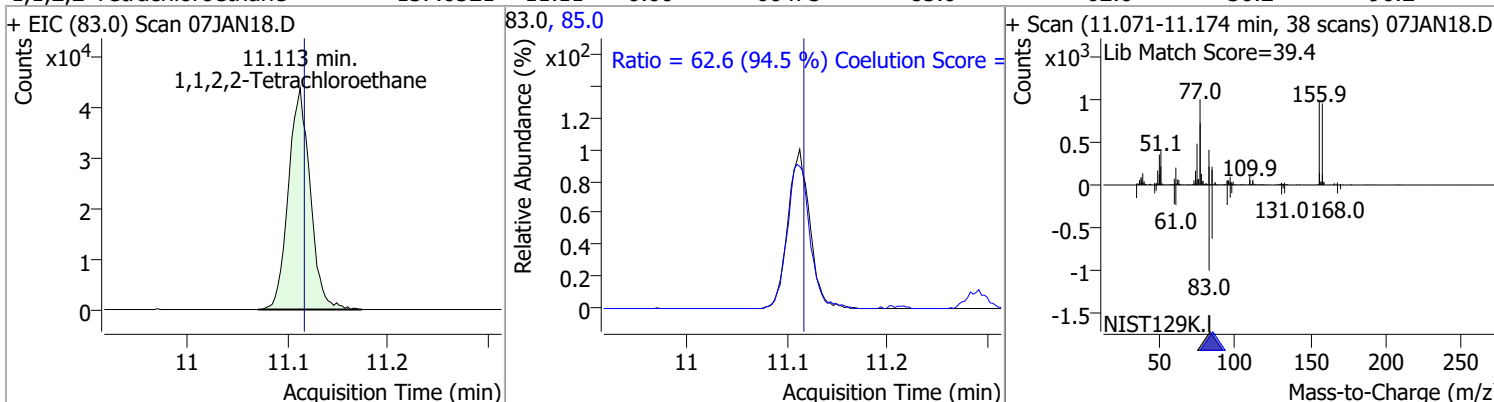










| Compound               | Conc.    | RT    | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|------------------------|----------|-------|----------|-------|-------|--------|-------|-------|
| 1,2,3-Trichloropropane | 134.5721 | 11.15 | 0.00     | 17465 | 112.0 | 62.5   | 33.5  | 93.5  |

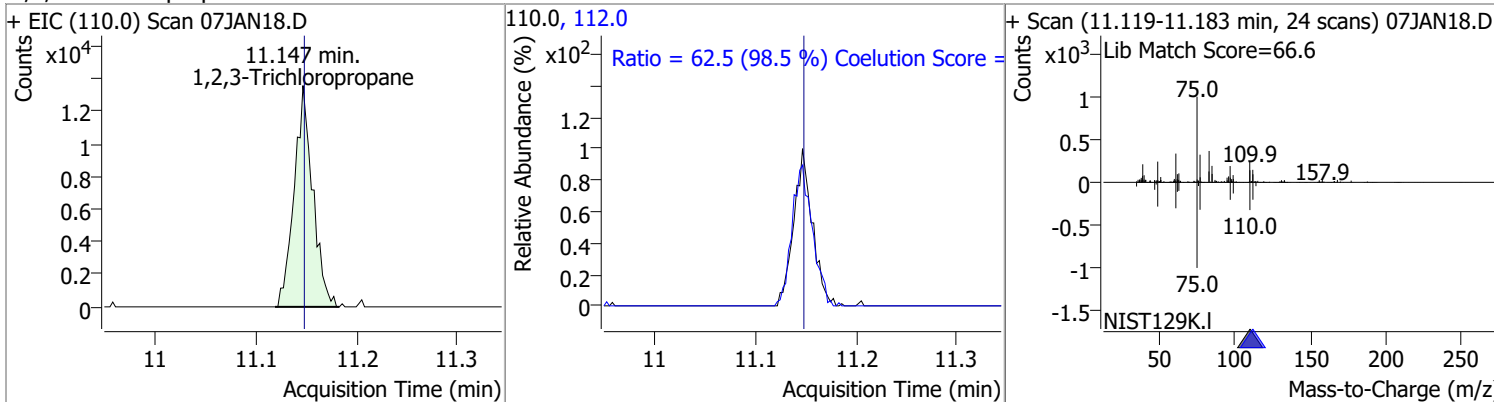

| Compound        | Conc.    | RT    | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|-----------------|----------|-------|----------|--------|------|--------|-------|-------|
| 2-Chlorotoluene | 141.2126 | 11.29 | 0.00     | 118405 | 91.0 | 282.4  | 252.3 | 312.3 |

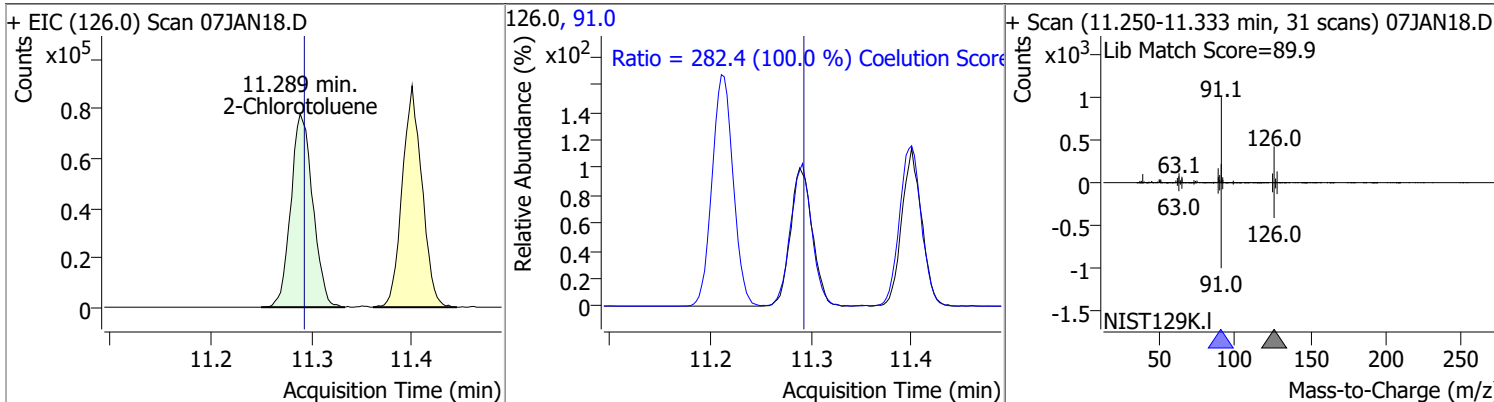




# Quantitation Results Report (QT Reviewed)
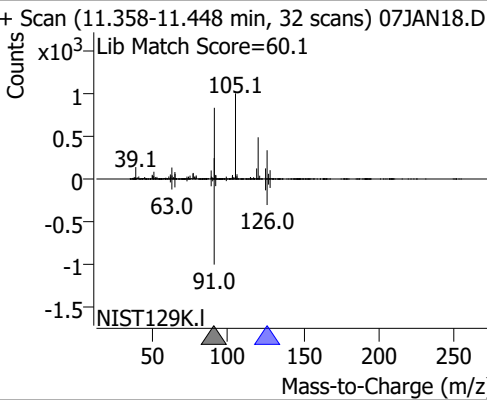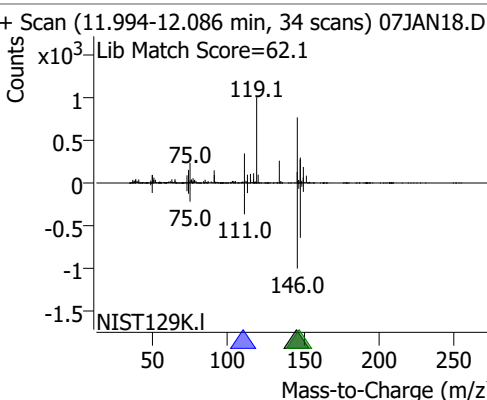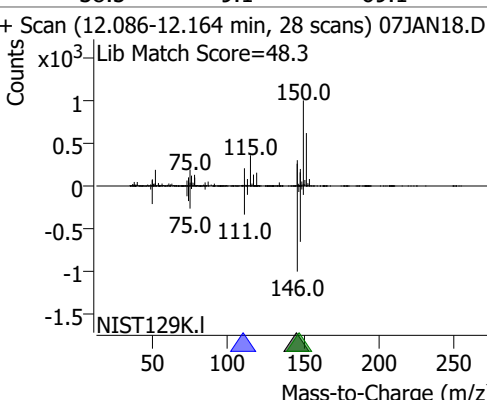
| Compound                                                                           | Conc.    | RT    | Dev(Min)                                                                             | Resp.  | QIon  | QRatio                                                                                | Lower | Upper |
|------------------------------------------------------------------------------------|----------|-------|--------------------------------------------------------------------------------------|--------|-------|---------------------------------------------------------------------------------------|-------|-------|
| 4-Chlorotoluene                                                                    | 142.0473 | 11.40 | 0.00                                                                                 | 388335 | 126.0 | 31.5                                                                                  | 1.7   | 61.7  |
|    |          |       |    |        |       |    |       |       |
| 1,3-Dichlorobenzene                                                                | 137.9499 | 12.03 | 0.00                                                                                 | 212018 | 148.0 | 63.8                                                                                  | 33.6  | 93.6  |
|   |          |       |   |        |       |   |       |       |
| 1,4-Dichlorobenzene                                                                | 137.4287 | 12.12 | 0.00                                                                                 | 215367 | 148.0 | 63.9                                                                                  | 33.1  | 93.1  |
|  |          |       |  |        |       |  |       |       |




# Quantitation Results Report (QT Reviewed)

| Compound            | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,2-Dichlorobenzene | 132.9681 | 12.49 | 0.00     | 172710 | 148.0 | 64.4   | 33.9  | 93.9  |
|                     |          |       |          |        | 111.0 | 40.7   | 11.0  | 71.0  |



# Quantitation Results Report (QT Reviewed)

|                |                                     |                   |                       |
|----------------|-------------------------------------|-------------------|-----------------------|
| Data File      | 07JAN20.D                           | Operator          | MSC                   |
| Acq. Method    | 5975CACQF.M                         | Acq. Date-Time    | 1/7/2022 6:29:09 PM   |
| Sample Name    | CCV010722_Closing                   | Instrument        | VOA5975C              |
| Vial           | 20                                  | Multiplier        | 1.00                  |
| DA Method File | VOA5975C_8260B_SHT_DoD_L4_010422.m  | Comment           |                       |
| Tune File      | BFB_Atune3.u                        | Tune Date         | 10/11/2021 4:02:00 PM |
| Batch Name     | VG010722_8260B.batch.bin            | Last Calib Update | 3/2/2022 10:41:44 AM  |
| Ref Library    | \\MASSHUNTER\Org\Library\NIST129K.I |                   |                       |

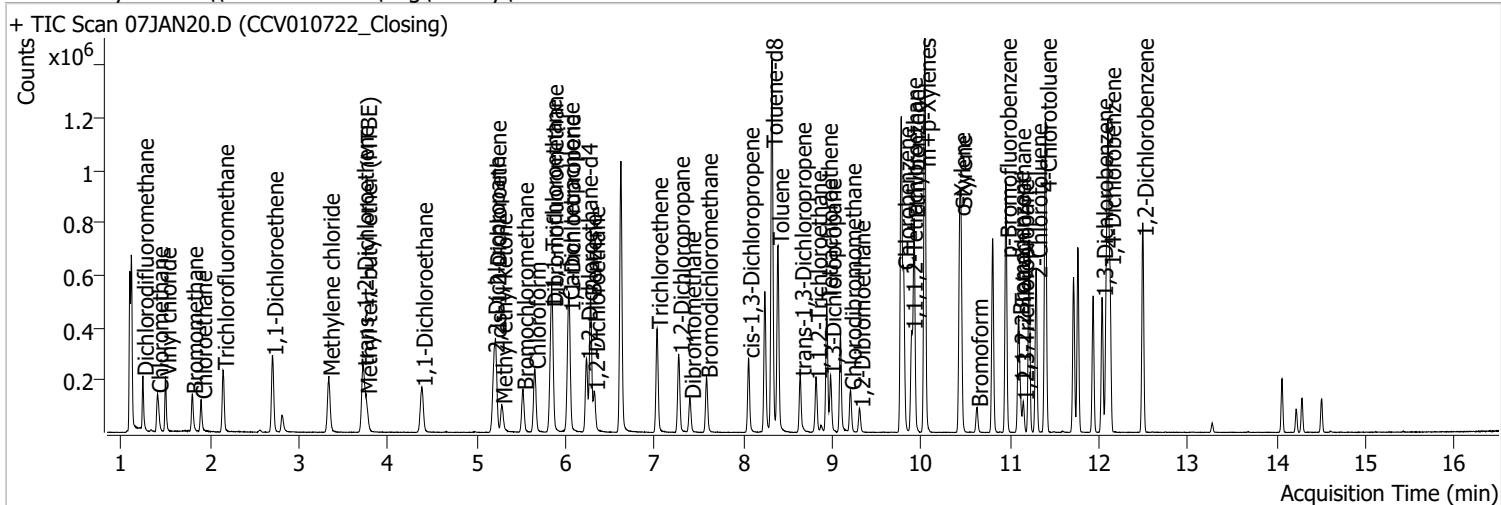

| Compound                           | RT                   | QIon  | Resp.  | Conc.              | Units | Dev(Min) |
|------------------------------------|----------------------|-------|--------|--------------------|-------|----------|
| <b>Internal Standards</b>          |                      |       |        |                    |       |          |
| M Fluorobenzene                    | 6.621                | 96.0  | 875212 | 250.0000           | ng    | -0.003   |
| M Chlorobenzene-d5                 | 9.775                | 82.0  | 332712 | 250.0000           | ng    | 0.003    |
| M 1,4-Dichlorobenzene-d4           | 12.100               | 152.0 | 273694 | 250.0000           | ng    | 0.000    |
| <b>System Monitoring Compounds</b> |                      |       |        |                    |       |          |
| S Dibromofluoromethane             | 5.851                | 113.0 | 220533 | 267.4624           | ng    | 0.006    |
| Spiked Amount: 250.000             | Range: 80.0 - 119.0% |       |        | Recovery = 106.98% |       |          |
| S 1,2-Dichloroethane-d4            | 6.236                | 67.0  | 97554  | 273.9195           | ng    | 0.003    |
| Spiked Amount: 250.000             | Range: 81.0 - 118.0% |       |        | Recovery = 109.57% |       |          |
| S Toluene-d8                       | 8.319                | 98.0  | 873247 | 272.3635           | ng    | 0.000    |
| Spiked Amount: 250.000             | Range: 89.0 - 112.0% |       |        | Recovery = 108.95% |       |          |
| S p-Bromofluorobenzene             | 10.951               | 95.0  | 269134 | 268.4143           | ng    | -0.003   |
| Spiked Amount: 250.000             | Range: 85.0 - 114.0% |       |        | Recovery = 107.37% |       |          |
| <b>Target Compounds</b>            |                      |       |        |                    |       |          |
| T Dichlorodifluoromethane          | 1.244                | 85.0  | 131556 | 114.7051           | ng    | 100      |
| T Chloromethane                    | 1.409                | 50.0  | 159080 | 114.2765           | ng    | 99       |
| T Vinyl chloride                   | 1.498                | 62.0  | 147497 | 117.7541           | ng    | 98       |
| T Bromomethane                     | 1.799                | 96.0  | 69603  | 124.2700           | ng    | 98       |
| T Chloroethane                     | 1.899                | 64.0  | 75250  | 121.3507           | ng    | 98       |
| T Trichlorofluoromethane           | 2.148                | 101.0 | 163895 | 105.4169           | ng    | 98       |
| T 1,1-Dichloroethene               | 2.700                | 96.0  | 104720 | 118.7865           | ng    | 100      |
| T Methylene chloride               | 3.336                | 49.0  | 149219 | 114.8197           | ng    | 98       |
| T trans-1,2-Dichloroethene         | 3.718                | 96.0  | 108710 | 120.8683           | ng    | 97       |
| T Methyl tert-butyl ether (MTBE)   | 3.754                | 73.0  | 138605 | 119.2255           | ng    | 99       |
| T 1,1-Dichloroethane               | 4.381                | 63.0  | 209364 | 125.0569           | ng    | 98       |
| T 2,2-Dichloropropane              | 5.193                | 77.0  | 152733 | 121.7521           | ng    | 99       |
| T cis-1,2-Dichloroethene           | 5.210                | 96.0  | 111394 | 122.1596           | ng    | 99       |
| T Methyl ethyl ketone              | 5.279                | 43.0  | 144340 | 1168.5921          | ng    | 100      |
| T Bromochloromethane               | 5.516                | 128.0 | 43567  | 115.3287           | ng    | 95       |
| T Chloroform                       | 5.653                | 83.0  | 197264 | 118.3968           | ng    | 96       |


# Quantitation Results Report (QT Reviewed)

| Compound                    | RT     | QIon  | Resp.  | Conc.    | Units | Dev(Min) |
|-----------------------------|--------|-------|--------|----------|-------|----------|
| T 1,1,1-Trichloroethane     | 5.834  | 97.0  | 185675 | 118.9139 | ng    | 99       |
| T Carbon tetrachloride      | 6.029  | 117.0 | 180946 | 117.6182 | ng    | 98       |
| T 1,1-Dichloropropene       | 6.043  | 75.0  | 159136 | 119.8660 | ng    | 99       |
| T Benzene                   | 6.280  | 78.0  | 426971 | 122.5270 | ng    | 99       |
| T 1,2-Dichloroethane        | 6.319  | 62.0  | 108503 | 115.0977 | ng    | 96       |
| T Trichloroethene           | 7.028  | 95.0  | 122705 | 122.2872 | ng    | 99       |
| T 1,2-Dichloropropane       | 7.270  | 63.0  | 109262 | 123.7897 | ng    | 98       |
| T Dibromomethane            | 7.399  | 93.0  | 45080  | 120.8597 | ng    | 96       |
| T Bromodichloromethane      | 7.585  | 83.0  | 121732 | 118.2568 | ng    | 96       |
| T cis-1,3-Dichloropropene   | 8.057  | 75.0  | 138637 | 119.1185 | ng    | 99       |
| T Toluene                   | 8.389  | 92.0  | 268266 | 123.8661 | ng    | 98       |
| T trans-1,3-Dichloropropene | 8.640  | 75.0  | 103086 | 124.4317 | ng    | 99       |
| T 1,1,2-Trichloroethane     | 8.818  | 83.0  | 50481  | 116.9843 | ng    | 99       |
| T Tetrachloroethene         | 8.935  | 163.8 | 105808 | 119.7520 | ng    | 98       |
| T 1,3-Dichloropropane       | 8.980  | 76.0  | 103169 | 121.5491 | ng    | 99       |
| T Chlorodibromomethane      | 9.203  | 129.0 | 79716  | 118.1999 | ng    | 98       |
| T 1,2-Dibromoethane         | 9.303  | 107.0 | 56624  | 120.0089 | ng    | 94       |
| T Chlorobenzene             | 9.802  | 112.0 | 287084 | 121.0758 | ng    | 99       |
| T 1,1,1,2-Tetrachloroethane | 9.892  | 131.0 | 96577  | 116.5186 | ng    | 97       |
| T Ethylbenzene              | 9.920  | 91.0  | 500217 | 121.6392 | ng    | 99       |
| T m+p-Xylenes               | 10.039 | 106.0 | 396787 | 248.2876 | ng    | 99       |
| T o-Xylene                  | 10.430 | 106.0 | 175221 | 123.1636 | ng    | 100      |
| T Styrene                   | 10.447 | 104.0 | 289229 | 126.2715 | ng    | 100      |
| T Bromoform                 | 10.628 | 172.5 | 42320  | 120.8329 | ng    | 99       |
| T Bromobenzene              | 11.094 | 156.0 | 110486 | 124.7379 | ng    | 98       |
| T 1,1,2,2-Tetrachloroethane | 11.113 | 83.0  | 61840  | 121.3005 | ng    | 96       |
| T 1,2,3-Trichloropropane    | 11.147 | 110.0 | 15684  | 114.9765 | ng    | 96       |
| T 2-Chlorotoluene           | 11.294 | 126.0 | 109275 | 123.9909 | ng    | 98       |
| T 4-Chlorotoluene           | 11.400 | 91.0  | 363039 | 126.3413 | ng    | 99       |
| T 1,3-Dichlorobenzene       | 12.033 | 146.0 | 196110 | 121.3987 | ng    | 100      |
| T 1,4-Dichlorobenzene       | 12.123 | 146.0 | 198916 | 120.7629 | ng    | 98       |
| T 1,2-Dichlorobenzene       | 12.493 | 146.0 | 162097 | 118.7328 | ng    | 100      |


(#) = Qualifier Out of Range; (m) = Manual Integration; (+) = Area Summed; (\*) = Surrogate Percent Recovery Out of Range; (d): Zeroed Peak

# Quantitation Results Report (QT Reviewed)


| Compound                | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|-------------------------|----------|------|----------|--------|------|--------|-------|-------|
| Dichlorodifluoromethane | 114.7051 | 1.24 | 0.00     | 131556 | 87.0 | 32.4   | 2.3   | 62.3  |

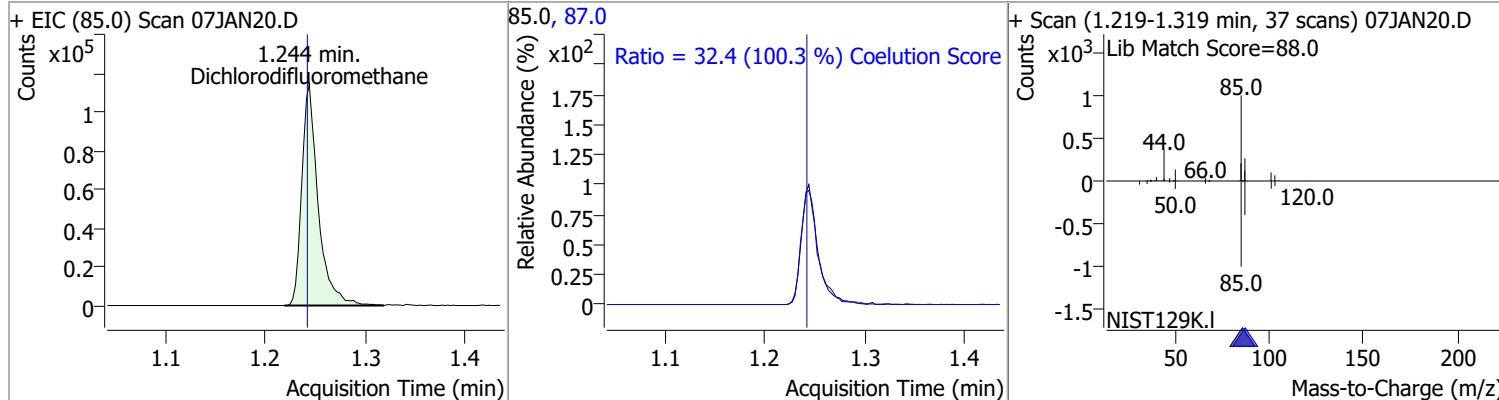


| Compound      | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------|----------|------|----------|--------|------|--------|-------|-------|
| Chloromethane | 114.2765 | 1.41 | 0.00     | 159080 | 52.0 | 32.9   | 2.1   | 62.1  |

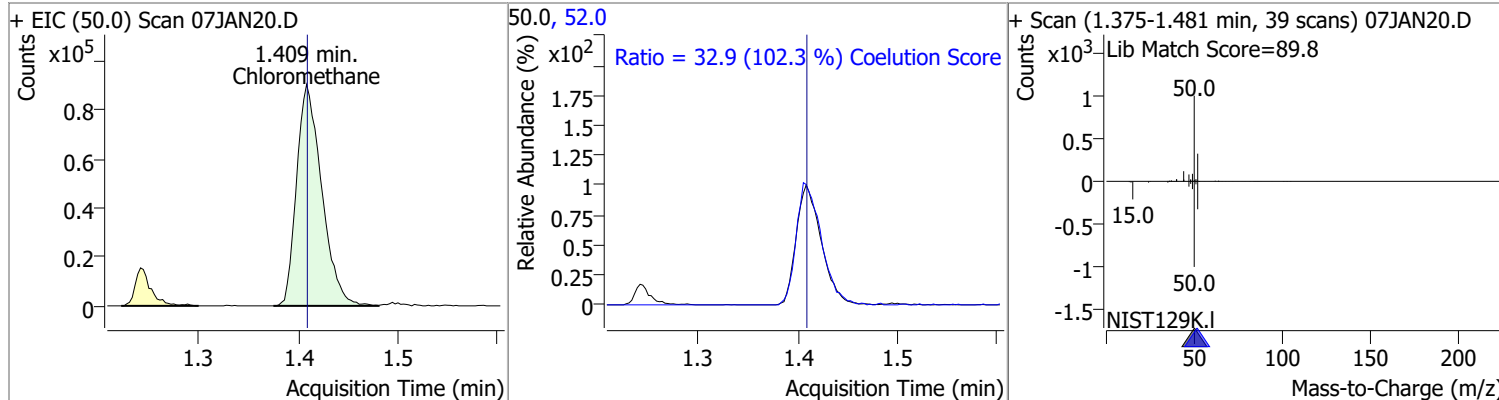

| Compound       | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|----------------|----------|------|----------|--------|------|--------|-------|-------|
| Vinyl chloride | 117.7541 | 1.50 | 0.00     | 147497 | 64.0 | 30.9   | 0.0   | 59.9  |

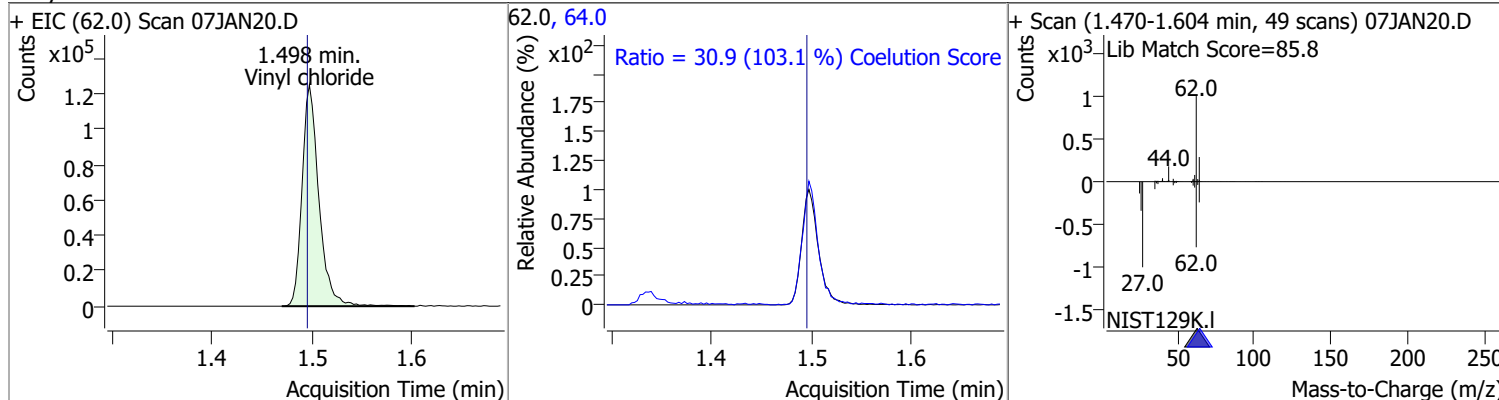


| Compound     | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|----------|------|----------|-------|------|--------|-------|-------|
| Bromomethane | 124.2700 | 1.80 | 0.00     | 69603 | 94.0 | 106.5  | 74.6  | 134.6 |

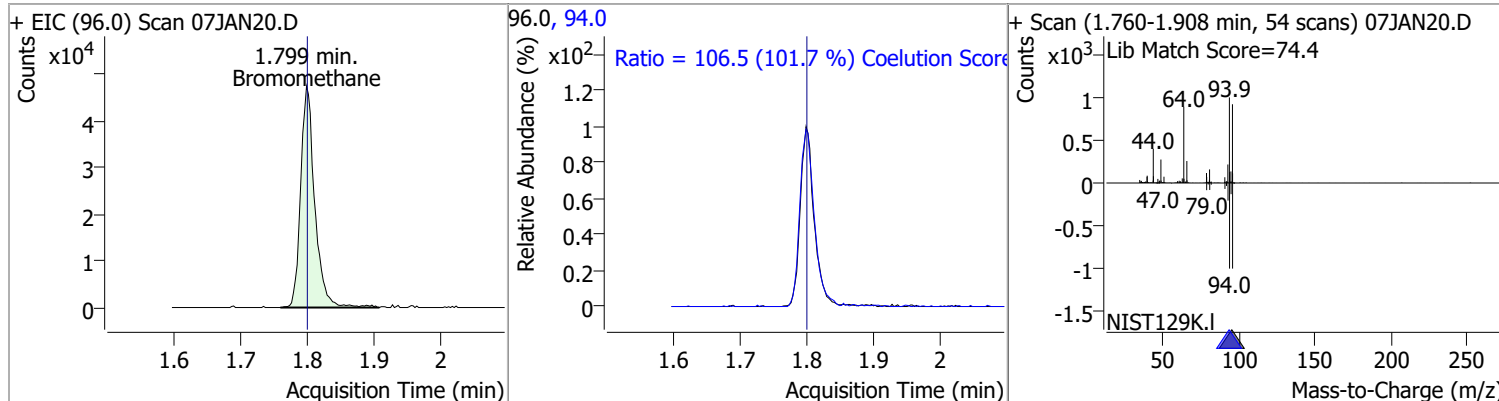


# Quantitation Results Report (QT Reviewed)


| Compound     | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------|----------|------|----------|-------|------|--------|-------|-------|
| Chloroethane | 121.3507 | 1.90 | 0.01     | 75250 | 66.0 | 31.3   | 0.1   | 60.1  |




| Compound               | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|------------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Trichlorofluoromethane | 105.4169 | 2.15 | 0.01     | 163895 | 103.0 | 65.5   | 34.2  | 94.2  |



| Compound           | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1-Dichloroethene | 118.7865 | 2.70 | 0.00     | 104720 | 61.0 | 180.0  | 150.3 | 210.3 |
|                    |          |      |          |        | 63.0 | 56.2   | 26.7  | 86.7  |




| Compound           | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| Methylene chloride | 114.8197 | 3.34 | 0.00     | 149219 | 84.0 | 67.7   | 36.9  | 96.9  |
|                    |          |      |          |        | 86.0 | 42.8   | 14.3  | 74.3  |




# Quantitation Results Report (QT Reviewed)


| Compound                 | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------------|----------|------|----------|--------|------|--------|-------|-------|
| trans-1,2-Dichloroethene | 120.8683 | 3.72 | 0.00     | 108710 | 61.0 | 157.4  | 123.9 | 183.9 |
|                          |          |      |          |        | 98.0 | 63.4   | 35.7  | 95.7  |



| Compound                       | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------------------|----------|------|----------|--------|------|--------|-------|-------|
| Methyl tert-butyl ether (MTBE) | 119.2255 | 3.75 | 0.00     | 138605 | 57.0 | 24.3   | 0.0   | 54.6  |




| Compound           | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,1-Dichloroethane | 125.0569 | 4.38 | 0.00     | 209364 | 65.0 | 30.9   | 2.1   | 62.1  |
|                    |          |      |          |        | 83.0 | 13.2   | 0.0   | 43.7  |




# Quantitation Results Report (QT Reviewed)


| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 2,2-Dichloropropane | 121.7521 | 5.19 | 0.00     | 152733 | 41.0 | 67.2   | 36.5  | 96.5  |
|                     |          |      |          |        | 97.0 | 22.7   | 0.0   | 53.2  |

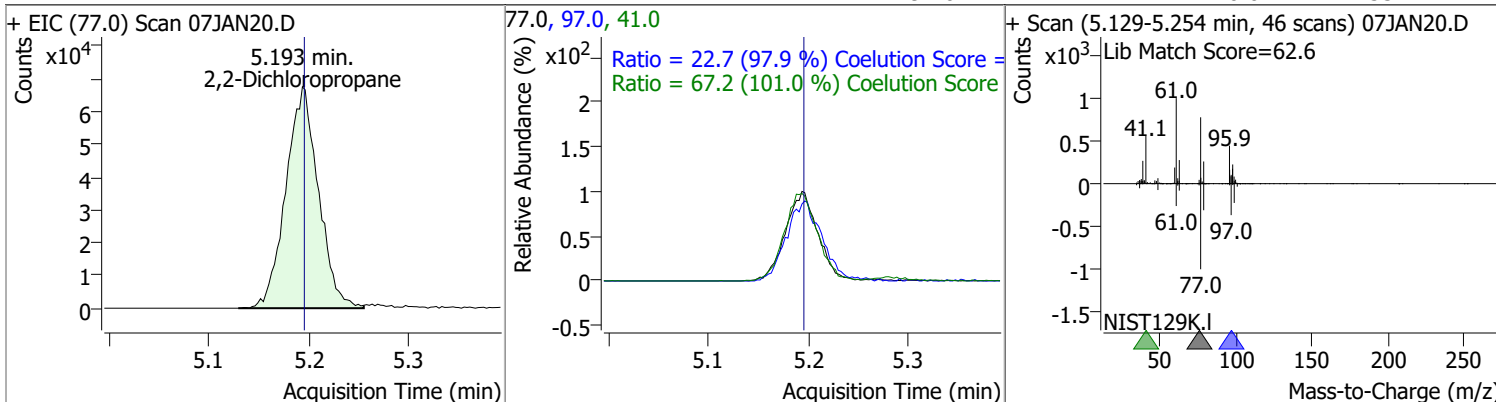


| Compound               | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,2-Dichloroethene | 122.1596 | 5.21 | -0.01    | 111394 | 61.0 | 164.9  | 137.2 | 197.2 |
|                        |          |      |          |        | 98.0 | 66.8   | 37.3  | 97.3  |

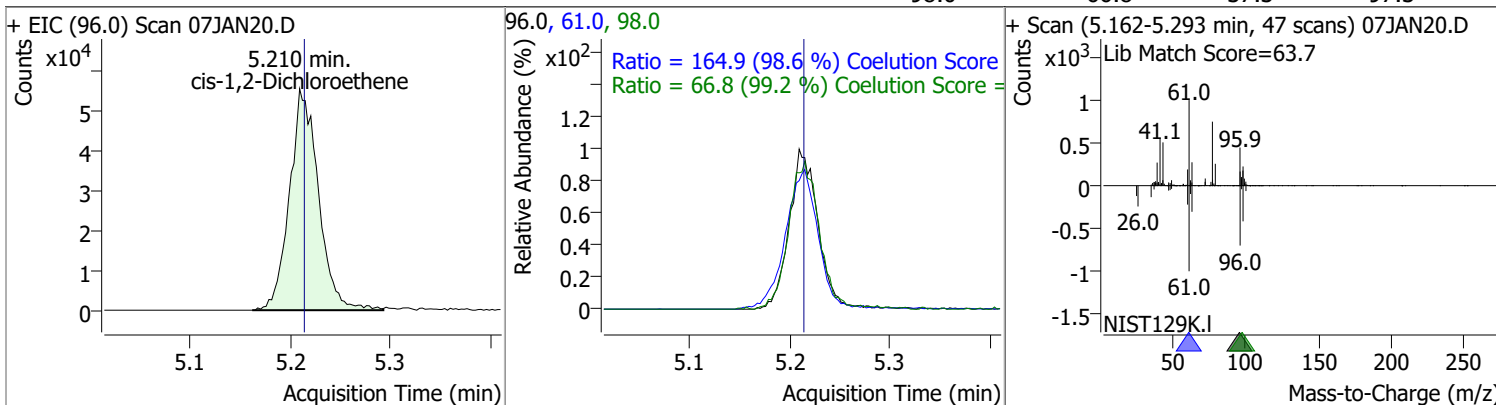

| Compound            | Conc.     | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|-----------|------|----------|--------|------|--------|-------|-------|
| Methyl ethyl ketone | 1168.5921 | 5.28 | 0.00     | 144340 | 72.0 | 21.1   | 0.0   | 51.3  |

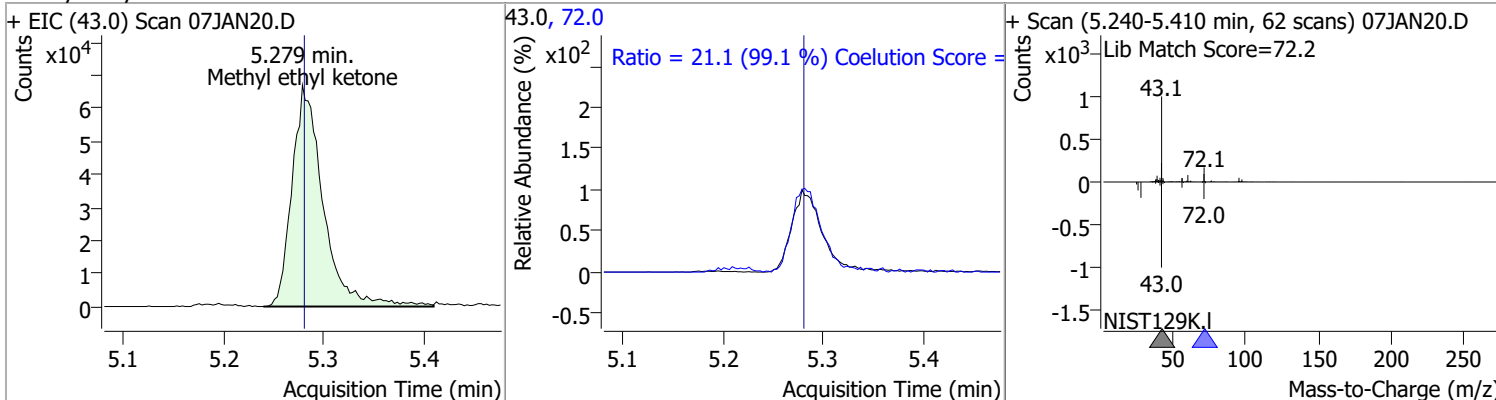


| Compound           | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|-------|------|--------|-------|-------|
| Bromochloromethane | 115.3287 | 5.52 | 0.00     | 43567 | 49.0 | 190.3  | 152.9 | 212.9 |

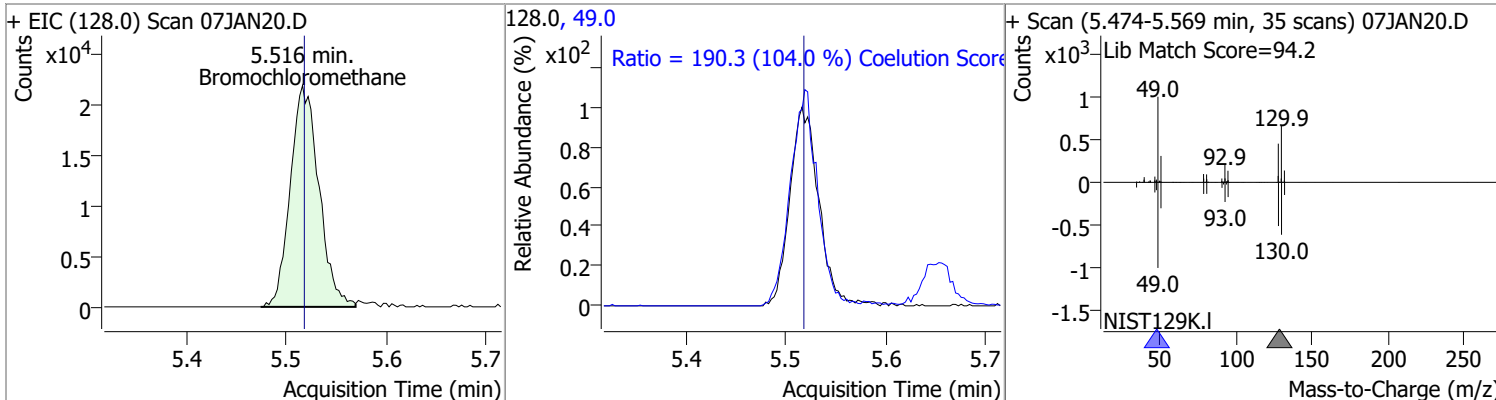


# Quantitation Results Report (QT Reviewed)


| Compound   | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|------|--------|-------|-------|
| Chloroform | 118.3968 | 5.65 | 0.00     | 197264 | 85.0 | 63.2   | 36.0  | 96.0  |




|                       |          |      |      |        |      |      |      |      |
|-----------------------|----------|------|------|--------|------|------|------|------|
| 1,1,1-Trichloroethane | 118.9139 | 5.83 | 0.00 | 185675 | 99.0 | 63.5 | 34.7 | 94.7 |
|                       |          |      |      |        | 61.0 | 47.6 | 18.1 | 78.1 |



|                      |          |      |      |        |       |      |     |      |
|----------------------|----------|------|------|--------|-------|------|-----|------|
| Dibromofluoromethane | 267.4624 | 5.85 | 0.01 | 220533 | 191.5 | 21.7 | 0.0 | 53.1 |
|----------------------|----------|------|------|--------|-------|------|-----|------|




|                      |          |      |      |        |       |      |      |       |
|----------------------|----------|------|------|--------|-------|------|------|-------|
| Carbon tetrachloride | 117.6182 | 6.03 | 0.01 | 180946 | 119.0 | 94.7 | 67.2 | 127.2 |
|                      |          |      |      |        | 121.0 | 31.4 | 0.1  | 60.1  |






# Quantitation Results Report (QT Reviewed)


| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|-------|--------|-------|-------|
| 1,1-Dichloropropene | 119.8660 | 6.04 | 0.01     | 159136 | 110.0 | 36.7   | 5.9   | 65.9  |
|                     |          |      |          |        | 77.0  | 30.8   | 0.1   | 60.1  |




| Compound              | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,2-Dichloroethane-d4 | 273.9195 | 6.24 | 0.00     | 97554 | 65.0 | 195.6  | 166.5 | 226.5 |



| Compound | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|----------|----------|------|----------|--------|------|--------|-------|-------|
| Benzene  | 122.5270 | 6.28 | 0.00     | 426971 | 77.0 | 23.8   | 0.0   | 53.5  |




| Compound           | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|--------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloroethane | 115.0977 | 6.32 | 0.00     | 108503 | 64.0 | 32.7   | 0.0   | 59.9  |
|                    |          |      |          |        | 98.0 | 8.1    | 0.0   | 37.6  |




# Quantitation Results Report (QT Reviewed)


| Compound        | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|-----------------|----------|------|----------|--------|-------|--------|-------|-------|
| Trichloroethene | 122.2872 | 7.03 | 0.00     | 122705 | 130.0 | 101.6  | 71.5  | 131.5 |
|                 |          |      |          |        | 97.0  | 62.6   | 34.1  | 94.1  |



| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,2-Dichloropropane | 123.7897 | 7.27 | 0.00     | 109262 | 76.0 | 37.3   | 8.2   | 68.2  |




| Compound       | Conc.    | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|----------------|----------|------|----------|-------|-------|--------|-------|-------|
| Dibromomethane | 120.8597 | 7.40 | 0.00     | 45080 | 173.5 | 106.4  | 83.7  | 143.7 |
|                |          |      |          |       | 95.0  | 82.5   | 52.2  | 112.2 |




# Quantitation Results Report (QT Reviewed)


| Compound             | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Bromodichloromethane | 118.2568 | 7.59 | 0.00     | 121732 | 85.0  | 67.8   | 34.5  | 94.5  |
|                      |          |      |          |        | 127.0 | 9.8    | 0.0   | 39.6  |



| Compound                | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|-------------------------|----------|------|----------|--------|------|--------|-------|-------|
| cis-1,3-Dichloropropene | 119.1185 | 8.06 | 0.00     | 138637 | 39.0 | 52.8   | 23.3  | 83.3  |
|                         |          |      |          |        | 77.0 | 31.7   | 1.0   | 61.0  |




| Compound   | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|------------|----------|------|----------|--------|-------|--------|-------|-------|
| Toluene-d8 | 272.3635 | 8.32 | 0.00     | 873247 | 100.0 | 64.1   | 34.4  | 94.4  |
|            |          |      |          |        | 99.0  | 9.6    | 0.0   | 39.6  |




# Quantitation Results Report (QT Reviewed)


| Compound | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|----------|----------|------|----------|--------|------|--------|-------|-------|
| Toluene  | 123.8661 | 8.39 | 0.00     | 268266 | 91.0 | 173.1  | 145.8 | 205.8 |



| Compound                  | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------------|----------|------|----------|--------|------|--------|-------|-------|
| trans-1,3-Dichloropropene | 124.4317 | 8.64 | 0.00     | 103086 | 39.0 | 52.5   | 23.4  | 83.4  |
|                           |          |      |          |        | 77.0 | 32.0   | 2.4   | 62.4  |

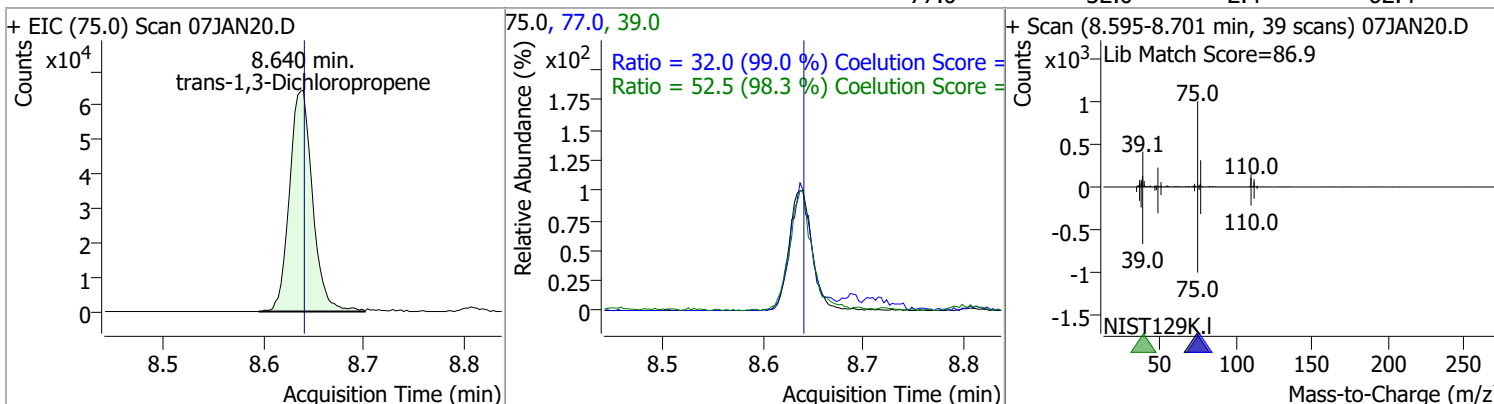


| Compound              | Conc.    | RT   | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|-----------------------|----------|------|----------|-------|------|--------|-------|-------|
| 1,1,2-Trichloroethane | 116.9843 | 8.82 | 0.00     | 50481 | 97.0 | 114.8  | 84.6  | 144.6 |
|                       |          |      |          |       | 85.0 | 65.4   | 37.6  | 97.6  |

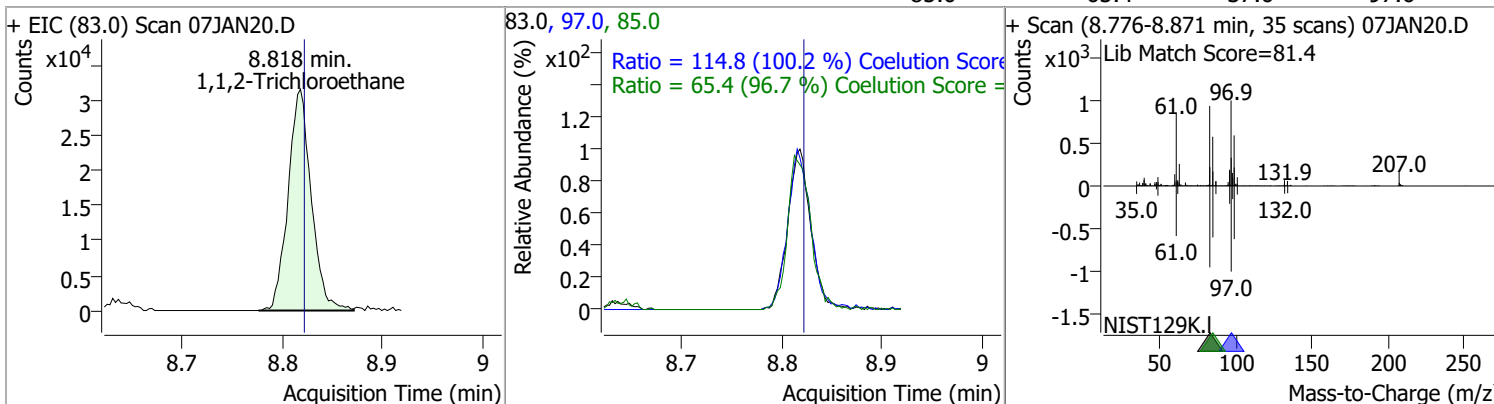


# Quantitation Results Report (QT Reviewed)


| Compound          | Conc.    | RT   | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|-------------------|----------|------|----------|--------|-------|--------|-------|-------|
| Tetrachloroethene | 119.7520 | 8.94 | 0.00     | 105808 | 165.8 | 125.6  | 98.6  | 158.6 |
|                   |          |      |          |        | 129.0 | 91.5   | 61.5  | 121.5 |

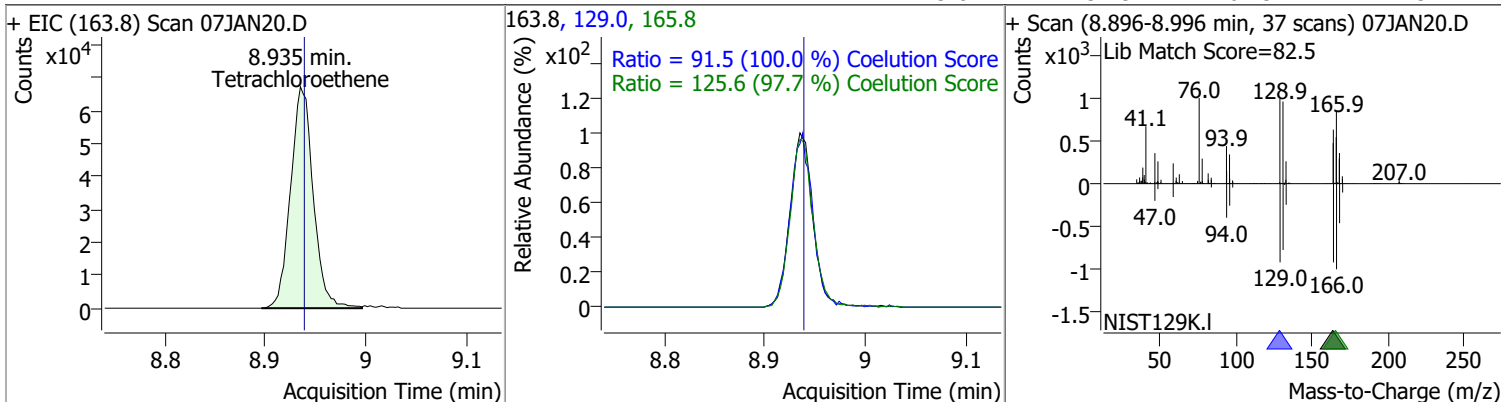


| Compound            | Conc.    | RT   | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|---------------------|----------|------|----------|--------|------|--------|-------|-------|
| 1,3-Dichloropropane | 121.5491 | 8.98 | 0.00     | 103169 | 78.0 | 32.6   | 2.9   | 62.9  |







| Compound             | Conc.    | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|----------------------|----------|------|----------|-------|-------|--------|-------|-------|
| Chlorodibromomethane | 118.1999 | 9.20 | 0.00     | 79716 | 127.0 | 76.3   | 48.0  | 108.0 |



| Compound          | Conc.    | RT   | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|-------------------|----------|------|----------|-------|-------|--------|-------|-------|
| 1,2-Dibromoethane | 120.0089 | 9.30 | 0.00     | 56624 | 109.0 | 88.9   | 64.5  | 124.5 |




# Quantitation Results Report (QT Reviewed)

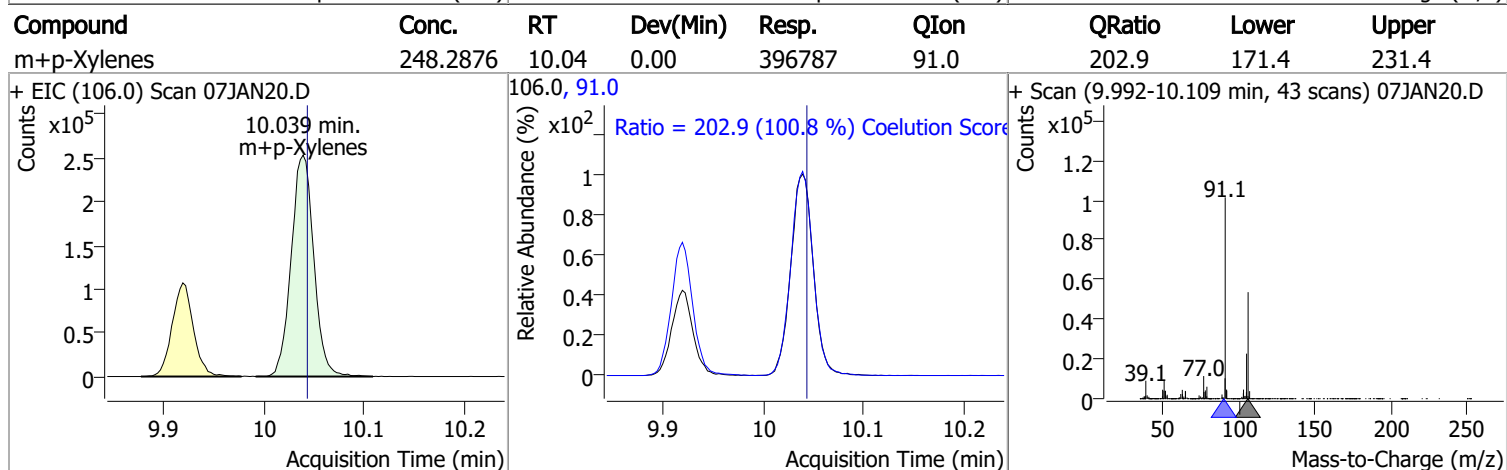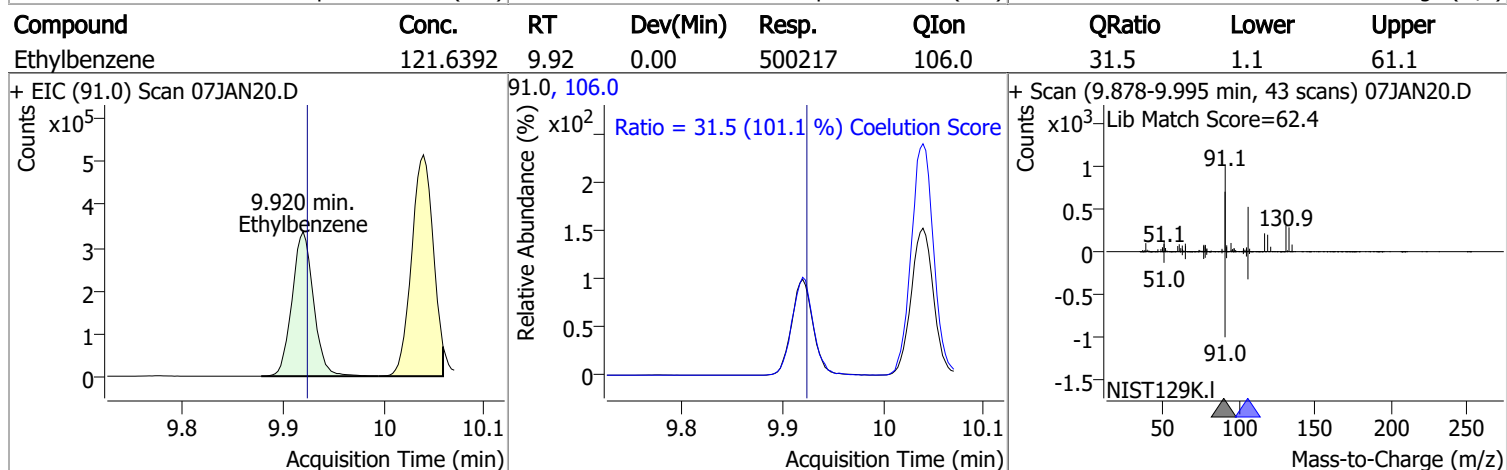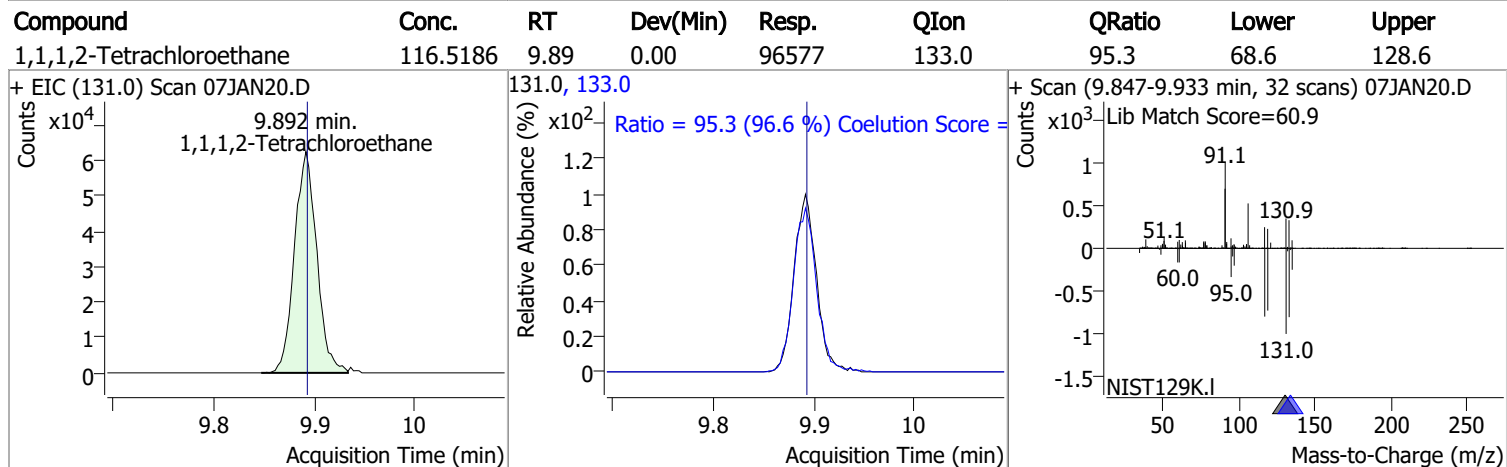


# Quantitation Results Report (QT Reviewed)


| Compound | Conc.    | RT    | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|----------|----------|-------|----------|--------|------|--------|-------|-------|
| o-Xylene | 123.1636 | 10.43 | 0.00     | 175221 | 91.0 | 213.8  | 183.1 | 243.1 |




| Compound | Conc.    | RT    | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|----------|----------|-------|----------|--------|------|--------|-------|-------|
| Styrene  | 126.2715 | 10.45 | 0.00     | 289229 | 78.0 | 49.3   | 19.6  | 79.6  |



| Compound  | Conc.    | RT    | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|-----------|----------|-------|----------|-------|-------|--------|-------|-------|
| Bromoform | 120.8329 | 10.63 | 0.00     | 42320 | 170.5 | 50.4   | 22.1  | 82.1  |
|           |          |       |          |       | 174.5 | 50.2   | 20.1  | 80.1  |




| Compound             | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|----------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| p-Bromofluorobenzene | 268.4143 | 10.95 | 0.00     | 269134 | 174.0 | 92.5   | 61.7  | 121.7 |
|                      |          |       |          |        | 176.0 | 91.1   | 60.6  | 120.6 |




# Quantitation Results Report (QT Reviewed)


| Compound     | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|--------------|----------|-------|----------|--------|-------|--------|-------|-------|
| Bromobenzene | 124.7379 | 11.09 | 0.00     | 110486 | 77.0  | 142.6  | 115.7 | 175.7 |
|              |          |       |          |        | 158.0 | 98.8   | 66.5  | 126.5 |

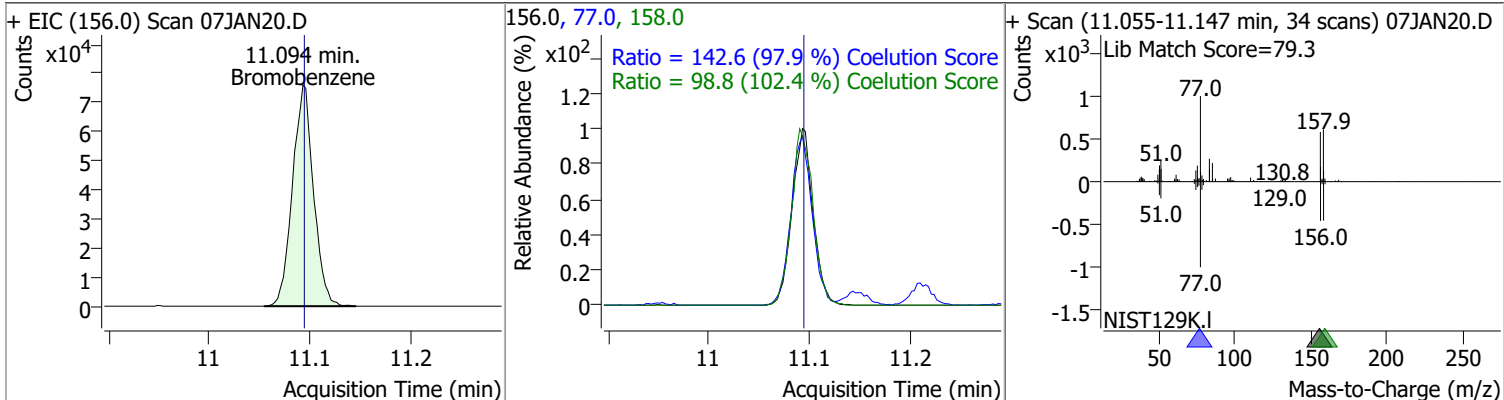


| Compound                  | Conc.    | RT    | Dev(Min) | Resp. | QIon | QRatio | Lower | Upper |
|---------------------------|----------|-------|----------|-------|------|--------|-------|-------|
| 1,1,2,2-Tetrachloroethane | 121.3005 | 11.11 | 0.00     | 61840 | 85.0 | 63.2   | 36.2  | 96.2  |

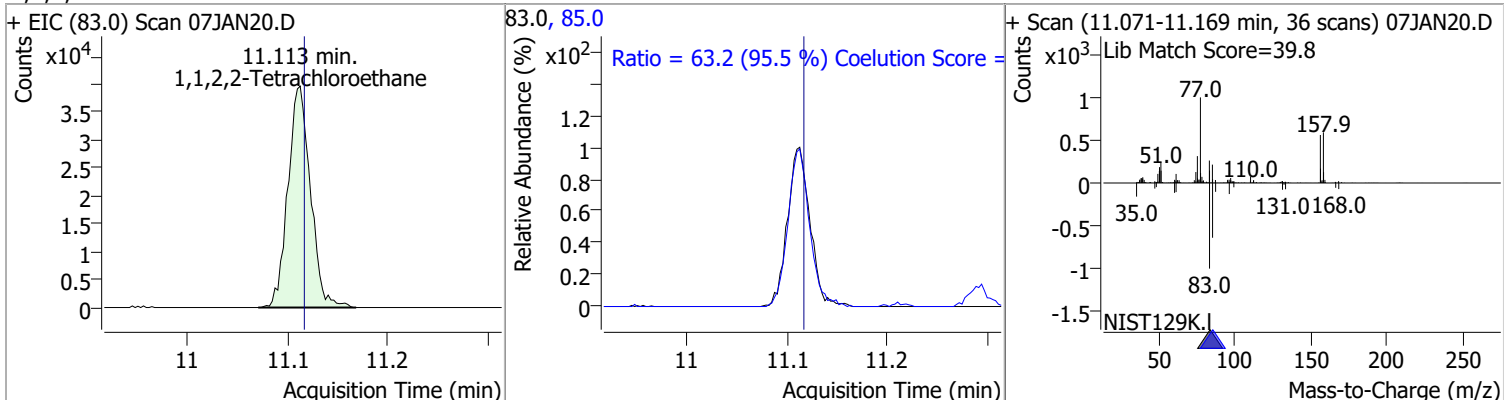

| Compound               | Conc.    | RT    | Dev(Min) | Resp. | QIon  | QRatio | Lower | Upper |
|------------------------|----------|-------|----------|-------|-------|--------|-------|-------|
| 1,2,3-Trichloropropane | 114.9765 | 11.15 | 0.00     | 15684 | 112.0 | 66.9   | 33.5  | 93.5  |









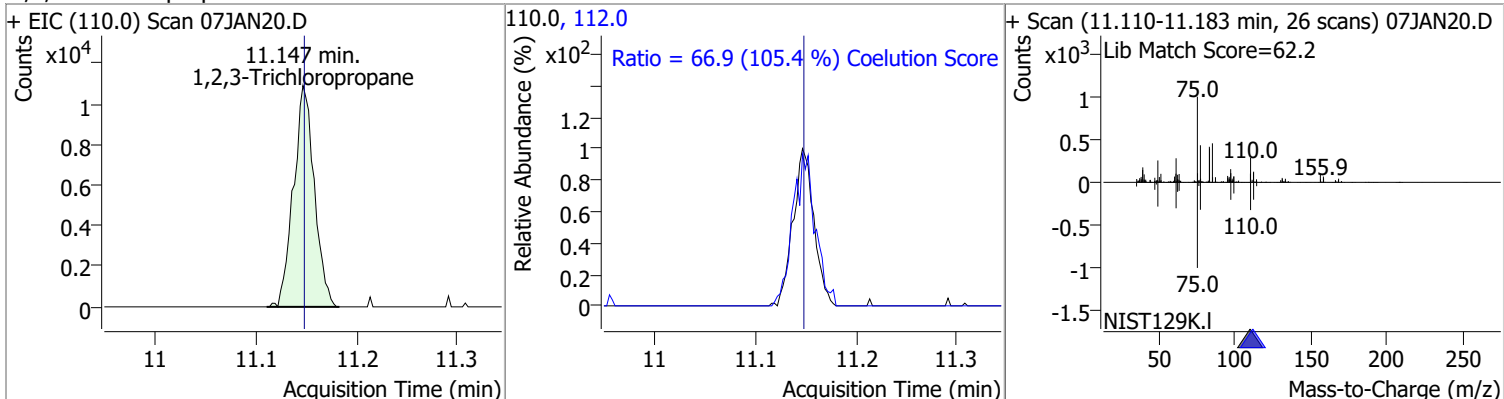


| Compound        | Conc.    | RT    | Dev(Min) | Resp.  | QIon | QRatio | Lower | Upper |
|-----------------|----------|-------|----------|--------|------|--------|-------|-------|
| 2-Chlorotoluene | 123.9909 | 11.29 | 0.00     | 109275 | 91.0 | 285.7  | 252.3 | 312.3 |

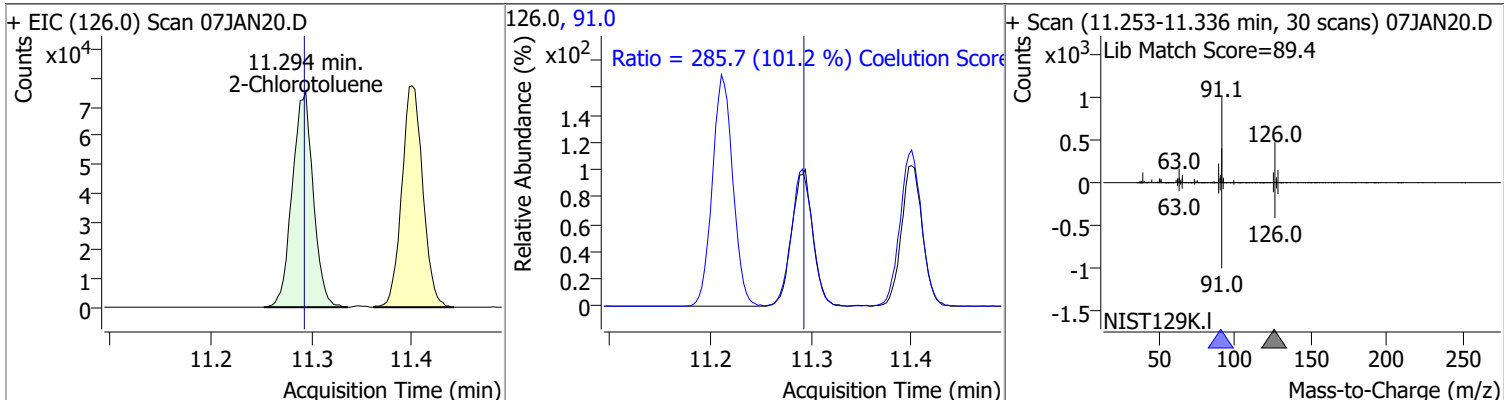






# Quantitation Results Report (QT Reviewed)

| Compound                                                                                                           | Conc.    | RT    | Dev(Min)                                                                                                    | Resp.  | QIon  | QRatio                                                                                                                                                          | Lower | Upper |
|--------------------------------------------------------------------------------------------------------------------|----------|-------|-------------------------------------------------------------------------------------------------------------|--------|-------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------|-------|-------|
| 4-Chlorotoluene                                                                                                    | 126.3413 | 11.40 | 0.00                                                                                                        | 363039 | 126.0 | 31.1                                                                                                                                                            | 1.7   | 61.7  |
| + EIC (91.0) Scan 07JAN20.D<br>    |          |       | 91.0, 126.0<br>           |        |       | + Scan (11.358-11.453 min, 35 scans) 07JAN20.D<br>Lib Match Score=58.2<br>   |       |       |
| 1,3-Dichlorobenzene                                                                                                | 121.3987 | 12.03 | 0.00                                                                                                        | 196110 | 148.0 | 63.6                                                                                                                                                            | 33.6  | 93.6  |
| + EIC (146.0) Scan 07JAN20.D<br>  |          |       | 146.0, 111.0, 148.0<br>  |        |       | + Scan (11.991-12.081 min, 33 scans) 07JAN20.D<br>Lib Match Score=68.0<br>  |       |       |
| 1,4-Dichlorobenzene                                                                                                | 120.7629 | 12.12 | 0.00                                                                                                        | 198916 | 148.0 | 64.6                                                                                                                                                            | 33.1  | 93.1  |
| + EIC (146.0) Scan 07JAN20.D<br> |          |       | 146.0, 111.0, 148.0<br> |        |       | + Scan (12.084-12.170 min, 32 scans) 07JAN20.D<br>Lib Match Score=47.1<br> |       |       |

# Quantitation Results Report (QT Reviewed)

| Compound            | Conc.    | RT    | Dev(Min) | Resp.  | QIon  | QRatio | Lower | Upper |
|---------------------|----------|-------|----------|--------|-------|--------|-------|-------|
| 1,2-Dichlorobenzene | 118.7328 | 12.49 | 0.00     | 162097 | 148.0 | 63.6   | 33.9  | 93.9  |
|                     |          |       |          |        | 111.0 | 40.9   | 11.0  | 71.0  |



# Audit Trail report

**Batch name and path:** D:\Org\Data\VOA5975C\VG010722\QuantResults\VG010722\_8260B.batch.bin  
**Quant batch version:** 10.0  
**Quant reporting version:** 10.0

| Name                         | User           | Time                 | Action                                                                             | Reason | Comment | Succeed | Exception |
|------------------------------|----------------|----------------------|------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdNewBatchTable             | BL2000\mchavez | 1/7/2022 9:13:24 AM  | Create new batch<br>D:\Org\Data\VOA5975C\VG010722\VG010722_8260B.batch.bin         |        |         | ✓       |           |
| CmdImportSamplesFromWorklist | BL2000\mchavez | 1/7/2022 9:13:32 AM  | Add samples from worklist:<br>D:\Org\Data\VOA5975C\VG010722\07JAN01.D              |        |         | ✓       |           |
| CmdStartMethodEditing        | BL2000\mchavez | 1/7/2022 9:14:04 AM  | Start method editing                                                               |        |         | ✓       |           |
| CmdImportMethodFromBatch     | BL2000\mchavez | 1/7/2022 9:14:05 AM  | Import method from batch<br>D:\Org\Data\VOA5975C\VG010622\VG010622_8260B.batch.bin |        |         | ✓       |           |
| CmdApplyMethodToAllSamples   | BL2000\mchavez | 1/7/2022 9:14:10 AM  | Apply method to all samples                                                        |        |         | ✓       |           |
| CmdMethodClear               | BL2000\mchavez | 1/7/2022 9:14:10 AM  | Clear method                                                                       |        |         | ✓       |           |
| CmdEndMethodEditing          | BL2000\mchavez | 1/7/2022 9:14:11 AM  | End method editing                                                                 |        |         | ✓       |           |
| CmdQuantitate                | BL2000\mchavez | 1/7/2022 9:14:14 AM  | Quantitate all compounds in all samples                                            |        |         | ✓       |           |
| CmdSaveBatchTable            | BL2000\mchavez | 1/7/2022 9:24:01 AM  | Save batch<br>D:\Org\Data\VOA5975C\VG010722\QuantResults\VG010722_8260B.batch.bin  |        |         | ✓       |           |
| CmdImportSamplesFromWorklist | BL2000\mchavez | 1/7/2022 9:25:03 AM  | Add samples from worklist:<br>D:\Org\Data\VOA5975C\VG010722\07JAN02.D              |        |         | ✓       |           |
| CmdSetSampleAttribute        | BL2000\mchavez | 1/7/2022 9:25:07 AM  | Set SampleType = TuneCheck for sample 07JAN02.D; previous value = Sample           |        |         | ✓       |           |
| CmdSaveBatchTable            | BL2000\mchavez | 1/7/2022 9:26:45 AM  | Save batch<br>D:\Org\Data\VOA5975C\VG010722\QuantResults\VG010722_8260B.batch.bin  |        |         | ✓       |           |
| CmdOpenBatchTable            | BL2000\mchavez | 1/7/2022 10:31:59 AM | Open batch<br>D:\Org\Data\VOA5975C\VG010722\VG010722_8260B.batch.bin               |        |         | ✓       |           |
| CmdImportSamplesFromWorklist | BL2000\mchavez | 1/7/2022 10:32:17 AM | Add samples from worklist:<br>D:\Org\Data\VOA5975C\VG010722\07JAN03.D              |        |         | ✓       |           |
| CmdSetSampleAttribute        | BL2000\mchavez | 1/7/2022 10:32:20 AM | Set SampleType = CC for sample 07JAN03.D; previous value = Sample                  |        |         | ✓       |           |
| CmdSetSampleAttribute        | BL2000\mchavez | 1/7/2022 10:32:26 AM | Set LevelName = CC for sample 07JAN03.D; previous value =                          |        |         | ✓       |           |
| CmdQuantitate                | BL2000\mchavez | 1/7/2022 10:32:29 AM | Quantitate all compounds in all samples                                            |        |         | ✓       |           |
| CmdSaveBatchTable            | BL2000\mchavez | 1/7/2022 10:33:53 AM | Save batch<br>D:\Org\Data\VOA5975C\VG010722\QuantResults\VG010722_8260B.batch.bin  |        |         | ✓       |           |

# Audit Trail report

| Name                         | User           | Time                 | Action                                                                                                            | Reason | Comment | Succeed | Exception |
|------------------------------|----------------|----------------------|-------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdOpenBatchTable            | BL2000\mchavez | 1/7/2022 11:19:56 AM | Open batch<br>D:\Org\Data\VOA5975C\VG010722\VG010722_8260B.batch.bin                                              |        |         | ✓       |           |
| CmdImportSamplesFromWorklist | BL2000\mchavez | 1/7/2022 11:20:13 AM | Add samples from worklist:<br>D:\Org\Data\VOA5975C\VG010722\07JAN04.D                                             |        |         | ✓       |           |
| CmdSetSampleAttribute        | BL2000\mchavez | 1/7/2022 11:20:18 AM | Set SampleType = QC for sample 07JAN04.D; previous value = Sample                                                 |        |         | ✓       |           |
| CmdSetSampleAttribute        | BL2000\mchavez | 1/7/2022 11:20:22 AM | Set LevelName = QC for sample 07JAN04.D; previous value =                                                         |        |         | ✓       |           |
| CmdSetSampleAttribute        | BL2000\mchavez | 1/7/2022 11:20:25 AM | Set SampleInformation = LCSA for sample 07JAN04.D; previous value =                                               |        |         | ✓       |           |
| CmdQuantitate                | BL2000\mchavez | 1/7/2022 11:20:29 AM | Quantitate all compounds in all samples                                                                           |        |         | ✓       |           |
| CmdSaveBatchTable            | BL2000\mchavez | 1/7/2022 11:20:55 AM | Save batch<br>D:\Org\Data\VOA5975C\VG010722\QuantResults\VG010722_8260B.batch.bin                                 |        |         | ✓       |           |
| CmdOpenBatchTable            | BL2000\mchavez | 1/7/2022 11:55:20 AM | Open batch<br>D:\Org\Data\VOA5975C\VG010722\VG010722_8260B.batch.bin                                              |        |         | ✓       |           |
| CmdImportSamplesFromWorklist | BL2000\mchavez | 1/7/2022 11:56:57 AM | Add samples from worklist:<br>D:\Org\Data\VOA5975C\VG010722\07JAN05.D                                             |        |         | ✓       |           |
| CmdQuantitate                | BL2000\mchavez | 1/7/2022 11:57:04 AM | Quantitate all compounds in all samples                                                                           |        |         | ✓       |           |
| CmdSaveBatchTable            | BL2000\mchavez | 1/7/2022 11:57:25 AM | Save batch<br>D:\Org\Data\VOA5975C\VG010722\QuantResults\VG010722_8260B.batch.bin                                 |        |         | ✓       |           |
| CmdOpenBatchTable            | BL2000\mchavez | 1/7/2022 12:03:31 PM | Open batch<br>D:\Org\Data\VOA5975C\VG010722\VG010722_8260B.batch.bin                                              |        |         | ✓       |           |
| CmdImportSamplesFromWorklist | BL2000\mchavez | 1/7/2022 12:03:46 PM | Add samples from worklist:<br>D:\Org\Data\VOA5975C\VG010722\07JAN06.D                                             |        |         | ✓       |           |
| CmdQuantitate                | BL2000\mchavez | 1/7/2022 12:03:51 PM | Quantitate all compounds in all samples                                                                           |        |         | ✓       |           |
| CmdSetSampleAttribute        | BL2000\mchavez | 1/7/2022 12:04:34 PM | Set SampleType = Blank for sample 07JAN06.D; previous value = Sample                                              |        |         | ✓       |           |
| CmdQuantitate                | BL2000\mchavez | 1/7/2022 12:04:38 PM | Quantitate all compounds in all samples                                                                           |        |         | ✓       |           |
| CmdSaveBatchTable            | BL2000\mchavez | 1/7/2022 12:11:24 PM | Save batch<br>D:\Org\Data\VOA5975C\VG010722\QuantResults\VG010722_8260B.batch.bin                                 |        |         | ✓       |           |
| CmdImportSamplesFromWorklist | BL2000\mchavez | 1/7/2022 1:16:43 PM  | Add samples from worklist:<br>D:\Org\Data\VOA5975C\VG010722\07JAN08.D,<br>D:\Org\Data\VOA5975C\VG010722\07JAN07.D |        |         | ✓       |           |
| CmdQuantitate                | BL2000\mchavez | 1/7/2022 1:16:50 PM  | Quantitate all compounds in all samples                                                                           |        |         | ✓       |           |

# Audit Trail report

| Name                         | User           | Time                 | Action                                                                                                                                                        | Reason | Comment | Succeed | Exception |
|------------------------------|----------------|----------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdSaveBatchTable            | BL2000\mchavez | 1/7/2022 1:33:40 PM  | Save batch<br>D:\Org\Data\VOA5975C\VG010722\QuantResults\VG010722_8260B.batch.bin                                                                             |        |         | ✓       |           |
| CmdOpenBatchTable            | BL2000\mchavez | 1/7/2022 2:44:00 PM  | Open batch<br>D:\Org\Data\VOA5975C\VG010722\VG010722_8260B.batch.bin                                                                                          |        |         | ✓       |           |
| CmdImportSamplesFromWorklist | BL2000\mchavez | 1/7/2022 2:44:40 PM  | Add samples from worklist:<br>D:\Org\Data\VOA5975C\VG010722\07JAN11.D,<br>D:\Org\Data\VOA5975C\VG010722\07JAN10.D,<br>D:\Org\Data\VOA5975C\VG010722\07JAN09.D |        |         | ✓       |           |
| CmdQuantitate                | BL2000\mchavez | 1/7/2022 2:44:51 PM  | Quantitate all compounds in all samples                                                                                                                       |        |         | ✓       |           |
| CmdSaveBatchTable            | BL2000\mchavez | 1/7/2022 2:51:46 PM  | Save batch<br>D:\Org\Data\VOA5975C\VG010722\QuantResults\VG010722_8260B.batch.bin                                                                             |        |         | ✓       |           |
| CmdOpenBatchTable            | BL2000\mchavez | 1/7/2022 3:59:33 PM  | Open batch<br>D:\Org\Data\VOA5975C\VG010722\VG010722_8260B.batch.bin                                                                                          |        |         | ✓       |           |
| CmdImportSamplesFromWorklist | BL2000\mchavez | 1/7/2022 4:00:03 PM  | Add samples from worklist:<br>D:\Org\Data\VOA5975C\VG010722\07JAN14.D,<br>D:\Org\Data\VOA5975C\VG010722\07JAN13.D,<br>D:\Org\Data\VOA5975C\VG010722\07JAN12.D |        |         | ✓       |           |
| CmdQuantitate                | BL2000\mchavez | 1/7/2022 4:00:13 PM  | Quantitate all compounds in all samples                                                                                                                       |        |         | ✓       |           |
| CmdSaveBatchTable            | BL2000\mchavez | 1/7/2022 4:15:06 PM  | Save batch<br>D:\Org\Data\VOA5975C\VG010722\QuantResults\VG010722_8260B.batch.bin                                                                             |        |         | ✓       |           |
| CmdOpenBatchTable            | BL2000\mchavez | 1/7/2022 4:21:12 PM  | Open batch<br>D:\Org\Data\VOA5975C\VG010722\VG010722_8260B.batch.bin                                                                                          |        |         | ✓       |           |
| CmdImportSamplesFromWorklist | BL2000\mchavez | 1/7/2022 4:21:51 PM  | Add samples from worklist:<br>D:\Org\Data\VOA5975C\VG010722\07JAN15.D                                                                                         |        |         | ✓       |           |
| CmdQuantitate                | BL2000\mchavez | 1/7/2022 4:22:04 PM  | Quantitate all compounds in all samples                                                                                                                       |        |         | ✓       |           |
| CmdSaveBatchTable            | BL2000\mchavez | 1/7/2022 4:34:37 PM  | Save batch<br>D:\Org\Data\VOA5975C\VG010722\QuantResults\VG010722_8260B.batch.bin                                                                             |        |         | ✓       |           |
| CmdOpenBatchTable            | BL2000\mchavez | 1/9/2022 12:17:18 PM | Open batch<br>D:\Org\Data\VOA5975C\VG010722\VG010722_8260B.batch.bin                                                                                          |        |         | ✓       |           |

# Audit Trail report

| Name                         | User           | Time                 | Action                                                                                                                                                                                                                                                                                            | Reason | Comment | Succeed | Exception |
|------------------------------|----------------|----------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdImportSamplesFromWorklist | BL2000\mchavez | 1/9/2022 12:18:19 PM | Add samples from worklist:<br>D:\Org\Data\VOA5975C\VG010722\07JAN21.D,<br>D:\Org\Data\VOA5975C\VG010722\07JAN20.D,<br>D:\Org\Data\VOA5975C\VG010722\07JAN19.D,<br>D:\Org\Data\VOA5975C\VG010722\07JAN18.D,<br>D:\Org\Data\VOA5975C\VG010722\07JAN17.D,<br>D:\Org\Data\VOA5975C\VG010722\07JAN16.D |        |         | ✓       |           |
| CmdSetSampleAttribute        | BL2000\mchavez | 1/9/2022 12:19:03 PM | Set SampleType = CC for sample 07JAN20.D; previous value = Sample                                                                                                                                                                                                                                 |        |         | ✓       |           |
| CmdSetSampleAttribute        | BL2000\mchavez | 1/9/2022 12:19:10 PM | Set LevelName = CC for sample 07JAN20.D; previous value =                                                                                                                                                                                                                                         |        |         | ✓       |           |
| CmdQuantitate                | BL2000\mchavez | 1/9/2022 12:19:23 PM | Quantitate all compounds in all samples                                                                                                                                                                                                                                                           |        |         | ✓       |           |
| CmdSetSampleAttribute        | BL2000\mchavez | 1/9/2022 12:19:53 PM | Set SampleType = Matrix for sample 07JAN17.D; previous value = Sample                                                                                                                                                                                                                             |        |         | ✓       |           |
| CmdSetSampleAttribute        | BL2000\mchavez | 1/9/2022 12:19:58 PM | Set SampleType = MatrixDup for sample 07JAN18.D; previous value = Sample                                                                                                                                                                                                                          |        |         | ✓       |           |
| CmdSetSampleAttribute        | BL2000\mchavez | 1/9/2022 12:20:04 PM | Set SampleInformation = MatrixA for sample 07JAN17.D; previous value =                                                                                                                                                                                                                            |        |         | ✓       |           |
| CmdSetSampleAttribute        | BL2000\mchavez | 1/9/2022 12:20:08 PM | Set SampleInformation = MatrixA for sample 07JAN18.D; previous value =                                                                                                                                                                                                                            |        |         | ✓       |           |
| CmdSetSampleAttribute        | BL2000\mchavez | 1/9/2022 12:20:12 PM | Set MatrixSpikeGroup = 219 for sample 07JAN17.D; previous value =                                                                                                                                                                                                                                 |        |         | ✓       |           |
| CmdSetSampleAttribute        | BL2000\mchavez | 1/9/2022 12:20:14 PM | Set MatrixSpikeGroup = 219 for sample 07JAN18.D; previous value =                                                                                                                                                                                                                                 |        |         | ✓       |           |
| CmdSetSampleAttribute        | BL2000\mchavez | 1/9/2022 12:24:41 PM | Set MatrixSpikeGroup = 219 for sample 07JAN11.D; previous value =                                                                                                                                                                                                                                 |        |         | ✓       |           |
| CmdSaveBatchTable            | BL2000\mchavez | 1/9/2022 12:26:45 PM | Save batch<br>D:\Org\Data\VOA5975C\VG010722\QuantResults\VG010722_8260B.batch.bin                                                                                                                                                                                                                 |        |         | ✓       |           |
| CmdOpenBatchTable            | BL2000\mchavez | 1/9/2022 9:08:38 PM  | Open batch<br>D:\Org\Data\VOA5975C\VG010722\VG010722_8260B.batch.bin                                                                                                                                                                                                                              |        |         | ✓       |           |
| CmdStartMethodEditing        | BL2000\mchavez | 1/9/2022 9:08:59 PM  | Start method editing                                                                                                                                                                                                                                                                              |        |         | ✓       |           |
| CmdImportMethodFromFile      | BL2000\mchavez | 1/9/2022 9:09:00 PM  | Import method from file<br>\\MASSHUNTER\Org\Data\Methods\Quant\VOA5975C\VOA5975C_010422_CAL\VOA5975C_8260B_SHT_DoD_L4_010422.m                                                                                                                                                                    |        |         | ✓       |           |
| CmdApplyMethodToAllSamples   | BL2000\mchavez | 1/9/2022 9:09:10 PM  | Apply method to all samples                                                                                                                                                                                                                                                                       |        |         | ✓       |           |
| CmdMethodClear               | BL2000\mchavez | 1/9/2022 9:09:10 PM  | Clear method                                                                                                                                                                                                                                                                                      |        |         | ✓       |           |
| CmdEndMethodEditing          | BL2000\mchavez | 1/9/2022 9:09:11 PM  | End method editing                                                                                                                                                                                                                                                                                |        |         | ✓       |           |

# Audit Trail report

| Name                              | User           | Time                  | Action                                                                                                                                                                                                                                                                            | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|-----------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdQuantitate                     | BL2000\mchavez | 1/9/2022 9:09:23 PM   | Quantitate all compounds in all samples                                                                                                                                                                                                                                           |        |         | ✓       |           |
| CmdSaveBatchTable                 | BL2000\mchavez | 1/9/2022 9:14:28 PM   | Save batch<br>D:\Org\Data\VOA5975C\VG010722\QuantResults\VG010722_8260B.batch.bin                                                                                                                                                                                                 |        |         | ✓       |           |
| CmdOpenBatchTable                 | BL2000\mchavez | 1/11/2022 10:34:48 AM | Open batch<br>D:\Org\Data\VOA5975C\VG010722\VG010722_8260B.batch.bin                                                                                                                                                                                                              |        |         | ✓       |           |
| CmdStartMethodEditing             | BL2000\mchavez | 1/11/2022 10:35:03 AM | Start method editing                                                                                                                                                                                                                                                              |        |         | ✓       |           |
| CmdImportMethodFromFile           | BL2000\mchavez | 1/11/2022 10:35:04 AM | Import method from file<br>\\MASSHUNTER\Org\Data\Methods\Quant\VOA5975C\VOA5975C_010422_CAL\VOA5975C_8260B_SHT_DoD_L4_010422.m                                                                                                                                                    |        |         | ✓       |           |
| CmdApplyMethodToAllSamples        | BL2000\mchavez | 1/11/2022 10:35:12 AM | Apply method to all samples                                                                                                                                                                                                                                                       |        |         | ✓       |           |
| CmdMethodClear                    | BL2000\mchavez | 1/11/2022 10:35:12 AM | Clear method                                                                                                                                                                                                                                                                      |        |         | ✓       |           |
| CmdEndMethodEditing               | BL2000\mchavez | 1/11/2022 10:35:12 AM | End method editing                                                                                                                                                                                                                                                                |        |         | ✓       |           |
| CmdQuantitate                     | BL2000\mchavez | 1/11/2022 10:35:24 AM | Quantitate all compounds in all samples                                                                                                                                                                                                                                           |        |         | ✓       |           |
| CmdSaveBatchTable                 | BL2000\mchavez | 1/11/2022 10:35:53 AM | Save batch<br>D:\Org\Data\VOA5975C\VG010722\QuantResults\VG010722_8260B.batch.bin                                                                                                                                                                                                 |        |         | ✓       |           |
| CmdOpenBatchTable                 | BL2000\mchavez | 1/11/2022 3:58:37 PM  | Open batch<br>D:\Org\Data\VOA5975C\VG010722\VG010722_8260B.batch.bin                                                                                                                                                                                                              |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/11/2022 4:00:44 PM  | Set SampleApproved = True for sample 07JAN03.D; previous value = False                                                                                                                                                                                                            |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/11/2022 4:01:01 PM  | Manually integrate qualifier 57.0 of compound Methyl tert-butyl ether (MTBE) in sample 07JAN04.D, from x, y = 3.681, 0 to 3.809, 338, result = 38793; previous integration is from x, y = 3.745, 144 to 3.809, 338 and previous response = 25564.                                 |        |         | ✓       |           |
| CmdManuallyIntegrateDropBaseline  | BL2000\mchavez | 1/11/2022 4:01:06 PM  | Drop baseline for qualifier 57.0 of compound Methyl tert-butyl ether (MTBE) in sample 07JAN04.D to y = 0, new integration is from x, y = 3.681, 0 to 3.809, 0 and new response = 40094; previous integration is from x, y = 3.681, 0 to 3.809, 338 and previous response = 38793. |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/11/2022 4:01:44 PM  | Set SampleApproved = True for sample 07JAN04.D; previous value = False                                                                                                                                                                                                            |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/11/2022 4:03:47 PM  | Set SampleApproved = True for sample 07JAN06.D; previous value = False                                                                                                                                                                                                            |        |         | ✓       |           |

# Audit Trail report

| Name                              | User           | Time                 | Action                                                                                                                              | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|-------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/11/2022 4:04:04 PM | Manually integrate compound Methylene chloride in sample 07JAN06.D from x, y = 3.310, 0 to 3.377, 0; result = 1664                  |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/11/2022 4:04:06 PM | Set UserAnnotation = NI for compound Methylene chloride in sample 07JAN06.D; previous value =                                       |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/11/2022 4:04:08 PM | Manually integrate qualifier84.0 of compound Methylene chloride in sample 07JAN06.D from x, y = 3.299, 0 to 3.394, 0; result = 1299 |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/11/2022 4:04:10 PM | Manually integrate qualifier86.0 of compound Methylene chloride in sample 07JAN06.D from x, y = 3.285, 0 to 3.400, 0; result = 522  |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/11/2022 4:05:13 PM | Manually integrate compound Chloromethane in sample 07JAN07.D from x, y = 1.364, 0 to 1.450, 0; result = 1730                       |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/11/2022 4:05:20 PM | Manually integrate qualifier52.0 of compound Chloromethane in sample 07JAN07.D from x, y = 1.364, 0 to 1.450, 0; result = 574       |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/11/2022 4:06:09 PM | Set UserAnnotation = NI for compound Chloromethane in sample 07JAN07.D; previous value =                                            |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/11/2022 4:06:18 PM | Manually integrate compound Methylene chloride in sample 07JAN07.D from x, y = 3.282, 0 to 3.394, 0; result = 2222                  |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/11/2022 4:06:20 PM | Manually integrate qualifier84.0 of compound Methylene chloride in sample 07JAN07.D from x, y = 3.282, 0 to 3.419, 0; result = 1662 |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/11/2022 4:06:23 PM | Manually integrate qualifier86.0 of compound Methylene chloride in sample 07JAN07.D from x, y = 3.294, 0 to 3.388, 0; result = 1096 |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/11/2022 4:06:25 PM | Set UserAnnotation = NI for compound Methylene chloride in sample 07JAN07.D; previous value =                                       |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/11/2022 4:07:09 PM | Manually integrate compound Chloroform in sample 07JAN07.D from x, y = 5.617, 0 to 5.697, 0; result = 209                           |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/11/2022 4:07:11 PM | Manually integrate qualifier85.0 of compound Chloroform in sample 07JAN07.D from x, y = 5.619, 0 to 5.675, 0; result = 105          |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/11/2022 4:07:15 PM | Set UserAnnotation = NI for compound Chloroform in sample 07JAN07.D; previous value =                                               |        |         | ✓       |           |



# Audit Trail report

| Name                              | User           | Time                 | Action                                                                                                                                                                                            | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/11/2022 4:07:54 PM | Manually integrate compound Benzene in sample 07JAN07.D from x, y = 6.263, 0 to 6.305, 0; result = 144                                                                                            |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/11/2022 4:07:56 PM | Manually integrate qualifier 77.0 of compound Benzene in sample 07JAN07.D from x, y = 6.252, 0 to 6.328, 0; result = 26                                                                           |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/11/2022 4:08:01 PM | Set UserAnnotation = NI for compound Benzene in sample 07JAN07.D; previous value =                                                                                                                |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/11/2022 4:08:54 PM | Manually integrate compound Ethylbenzene in sample 07JAN07.D from x, y = 9.891, 0 to 9.953, 0; result = 389                                                                                       |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/11/2022 4:08:56 PM | Manually integrate qualifier 106.0 of compound Ethylbenzene in sample 07JAN07.D from x, y = 9.917, 0 to 9.958, 0; result = 37                                                                     |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/11/2022 4:08:58 PM | Set UserAnnotation = NI for compound Ethylbenzene in sample 07JAN07.D; previous value =                                                                                                           |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/11/2022 4:09:04 PM | Manually integrate compound m+p-Xylenes in sample 07JAN07.D from x, y = 10.009, 0 to 10.059, 0; result = 88                                                                                       |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/11/2022 4:09:06 PM | Manually integrate qualifier 91.0 of compound m+p-Xylenes in sample 07JAN07.D from x, y = 10.006, 0 to 10.078, 0; result = 443                                                                    |        |         | ✓       |           |
| CmdZeroOutPeak                    | BL2000\mchavez | 1/11/2022 4:09:08 PM | Zero out primary peak of compound Ethylbenzene in sample 07JAN07.D                                                                                                                                |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/11/2022 4:09:13 PM | Manually integrate compound Ethylbenzene in sample 07JAN07.D, from x, y = 9.903, 0 to 9.942, 0, result = 389; previous integration is from x, y = 9.917, 0 to 9.917, 0 and previous response = 0. |        |         | ✓       |           |
| CmdZeroOutPeak                    | BL2000\mchavez | 1/11/2022 4:09:17 PM | Zero out primary peak of compound m+p-Xylenes in sample 07JAN07.D                                                                                                                                 |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/11/2022 4:10:30 PM | Set SampleApproved = True for sample 07JAN07.D; previous value = False                                                                                                                            |        |         | ✓       |           |
| CmdQuantitate                     | BL2000\mchavez | 1/11/2022 4:10:42 PM | Quantitate all compounds in all samples                                                                                                                                                           |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/11/2022 4:11:11 PM | Set UserDefined = Qualifier ratio did not meet method criteria for m+p Xylenes for sample 07JAN07.D; previous value =                                                                             |        |         | ✓       |           |
| CmdSaveBatchTable                 | BL2000\mchavez | 1/11/2022 4:54:29 PM | Save batch<br>D:\Org\Data\VOA5975C\VG010722\QuantResults\VG010722_8260B.batch.bin                                                                                                                 |        |         | ✓       |           |

# Audit Trail report

| Name                              | User           | Time                 | Action                                                                                                                              | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|-------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdOpenBatchTable                 | BL2000\mchavez | 1/12/2022 9:04:15 AM | Open batch<br>D:\Org\Data\VOA5975C\VG010722\VG010722_8260B.batch.bin                                                                |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:04:32 AM | Manually integrate qualifier52.0 of compound Chloromethane in sample 07JAN08.D from x, y = 1.369, 0 to 1.445, 0; result = 737       |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:04:52 AM | Manually integrate qualifier84.0 of compound Methylene chloride in sample 07JAN08.D from x, y = 3.294, 0 to 3.391, 0; result = 1567 |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:04:56 AM | Manually integrate qualifier86.0 of compound Methylene chloride in sample 07JAN08.D from x, y = 3.294, 0 to 3.361, 0; result = 978  |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:05:17 AM | Manually integrate compound Benzene in sample 07JAN08.D from x, y = 6.264, 0 to 6.305, 0; result = 212                              |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/12/2022 9:05:19 AM | Set UserAnnotation = NI for compound Benzene in sample 07JAN08.D; previous value =                                                  |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:05:21 AM | Manually integrate qualifier77.0 of compound Benzene in sample 07JAN08.D from x, y = 6.264, 0 to 6.314, 0; result = 84              |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:05:53 AM | Manually integrate compound Ethylbenzene in sample 07JAN08.D from x, y = 9.903, 0 to 9.939, 0; result = 483                         |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:05:55 AM | Manually integrate qualifier106.0 of compound Ethylbenzene in sample 07JAN08.D from x, y = 9.900, 0 to 9.936, 0; result = 26        |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/12/2022 9:05:58 AM | Set UserAnnotation = NI for compound Ethylbenzene in sample 07JAN08.D; previous value =                                             |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:06:35 AM | Manually integrate compound m+p-Xylenes in sample 07JAN08.D from x, y = 10.014, 0 to 10.042, 0; result = 200                        |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:06:37 AM | Manually integrate qualifier91.0 of compound m+p-Xylenes in sample 07JAN08.D from x, y = 10.003, 0 to 10.064, 0; result = 712       |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/12/2022 9:06:41 AM | Set UserAnnotation = NI for compound m+p-Xylenes in sample 07JAN08.D; previous value =                                              |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/12/2022 9:06:44 AM | Set UserAnnotation = for compound m+p-Xylenes in sample 07JAN08.D; previous value = NI                                              |        |         | ✓       |           |
| CmdZeroOutPeak                    | BL2000\mchavez | 1/12/2022 9:06:47 AM | Zero out primary peak of compound m+p-Xylenes in sample 07JAN08.D                                                                   |        |         | ✓       |           |

# Audit Trail report

| Name                              | User           | Time                 | Action                                                                                                                                                                                                      | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdSetSampleAttribute             | BL2000\mchavez | 1/12/2022 9:07:09 AM | Set UserDefined = Qualifier ratio did not meet method criteria for m+p Xylenes for sample 07JAN08.D; previous value =                                                                                       |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/12/2022 9:07:32 AM | Set SampleApproved = True for sample 07JAN08.D; previous value = False                                                                                                                                      |        |         | ✓       |           |
| CmdQuantitate                     | BL2000\mchavez | 1/12/2022 9:07:50 AM | Quantitate all compounds in all samples                                                                                                                                                                     |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:09:43 AM | Manually integrate compound Chloroform in sample 07JAN09.D from x, y = 5.617, 0 to 5.689, 0; result = 381                                                                                                   |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:09:46 AM | Manually integrate qualifier85.0 of compound Chloroform in sample 07JAN09.D from x, y = 5.608, 0 to 5.675, 0; result = 250                                                                                  |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:10:07 AM | Manually integrate compound Methylene chloride in sample 07JAN09.D, from x, y = 3.274, 0 to 3.375, 0, result = 2658; previous integration is from x, y = 3.316, 0 to 3.375, 0 and previous response = 2339. |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/12/2022 9:10:09 AM | Set UserAnnotation = LT for compound Methylene chloride in sample 07JAN09.D; previous value =                                                                                                               |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:10:12 AM | Manually integrate qualifier84.0 of compound Methylene chloride in sample 07JAN09.D from x, y = 3.305, 0 to 3.386, 0; result = 1818                                                                         |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:10:14 AM | Manually integrate qualifier86.0 of compound Methylene chloride in sample 07JAN09.D from x, y = 3.305, 0 to 3.377, 0; result = 1137                                                                         |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:10:26 AM | Manually integrate compound Chloromethane in sample 07JAN09.D from x, y = 1.372, 0 to 1.456, 0; result = 1041                                                                                               |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:10:28 AM | Manually integrate qualifier52.0 of compound Chloromethane in sample 07JAN09.D from x, y = 1.367, 0 to 1.462, 0; result = 421                                                                               |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/12/2022 9:10:35 AM | Set UserAnnotation = NI for compound Chloromethane in sample 07JAN09.D; previous value =                                                                                                                    |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/12/2022 9:10:41 AM | Set UserAnnotation = NI for compound Chloroform in sample 07JAN09.D; previous value =                                                                                                                       |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/12/2022 9:10:44 AM | Set SampleApproved = True for sample 07JAN09.D; previous value = False                                                                                                                                      |        |         | ✓       |           |

# Audit Trail report

| Name                              | User           | Time                 | Action                                                                                                                                                                            | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:11:07 AM | Manually integrate qualifier52.0 of compound Chloromethane in sample 07JAN10.D from x, y = 1.381, 0 to 1.445, 0; result = 734                                                     |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:11:21 AM | Manually integrate compound Methylene chloride in sample 07JAN10.D from x, y = 3.291, 0 to 3.400, 0; result = 1975                                                                |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:11:23 AM | Manually integrate qualifier84.0 of compound Methylene chloride in sample 07JAN10.D from x, y = 3.291, 0 to 3.400, 0; result = 1289                                               |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:11:25 AM | Manually integrate qualifier86.0 of compound Methylene chloride in sample 07JAN10.D from x, y = 3.299, 0 to 3.414, 0; result = 796                                                |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/12/2022 9:11:28 AM | Set UserAnnotation = NI for compound Methylene chloride in sample 07JAN10.D; previous value =                                                                                     |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:11:40 AM | Manually integrate compound Chloroform in sample 07JAN10.D from x, y = 5.617, 0 to 5.689, 0; result = 53                                                                          |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:11:42 AM | Manually integrate qualifier85.0 of compound Chloroform in sample 07JAN10.D from x, y = 5.625, 0 to 5.709, 0; result = 110                                                        |        |         | ✓       |           |
| CmdZeroOutPeak                    | BL2000\mchavez | 1/12/2022 9:11:47 AM | Zero out primary peak of compound Chloroform in sample 07JAN10.D                                                                                                                  |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/12/2022 9:11:58 AM | Set UserDefined = Qualifier ratio did not meet method criteria for m+p Xylenes for sample 07JAN10.D; previous value =                                                             |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/12/2022 9:12:09 AM | Set UserDefined = Qualifier ratio did not meet method criteria for Chloroform for sample 07JAN10.D; previous value = Qualifier ratio did not meet method criteria for m+p Xylenes |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:12:31 AM | Manually integrate compound Benzene in sample 07JAN10.D from x, y = 6.250, 0 to 6.328, 0; result = 229                                                                            |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:12:32 AM | Manually integrate qualifier77.0 of compound Benzene in sample 07JAN10.D from x, y = 6.258, 0 to 6.319, 0; result = 33                                                            |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/12/2022 9:12:43 AM | Set UserAnnotation = NI for compound Benzene in sample 07JAN10.D; previous value =                                                                                                |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:12:53 AM | Manually integrate compound Bromodichloromethane in sample 07JAN10.D from x, y = 7.541, 0 to 7.633, 0; result = 903                                                               |        |         | ✓       |           |

# Audit Trail report

| Name                              | User           | Time                 | Action                                                                                                                                                                                                                                    | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:12:55 AM | Manually integrate qualifier 85.0 of compound Bromodichloromethane in sample 07JAN10.D from x, y = 7.544, 0 to 7.636, 0; result = 309                                                                                                     |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:12:57 AM | Manually integrate qualifier 127.0 of compound Bromodichloromethane in sample 07JAN10.D from x, y = 7.558, 0 to 7.630, 0; result = 35                                                                                                     |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:12:58 AM | Manually integrate qualifier 127.0 of compound Bromodichloromethane in sample 07JAN10.D, from x, y = 7.613, 0 to 7.630, 0, result = 0; previous integration is from x, y = 7.558, 0 to 7.630, 0 and previous response = 35.               |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:13:00 AM | Manually integrate qualifier 127.0 of compound Bromodichloromethane in sample 07JAN10.D, from x, y = 7.563, 0 to 7.599, 0, result = 35; previous integration is from x, y = 7.613, 0 to 7.630, 0 and previous response = 0.               |        |         | ✓       |           |
| CmdZeroOutPeak                    | BL2000\mchavez | 1/12/2022 9:13:05 AM | Zero out primary peak of compound Bromodichloromethane in sample 07JAN10.D                                                                                                                                                                |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/12/2022 9:13:26 AM | Set UserDefined = Qualifier ratio did not meet method criteria for Chloroform, Bromodichloromethane for sample 07JAN10.D; previous value = Qualifier ratio did not meet method criteria for Chloroform                                    |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:13:44 AM | Manually integrate compound Chlorodibromomethane in sample 07JAN10.D, from x, y = 9.172, 0 to 9.253, 0, result = 5690; previous integration is from x, y = 9.172, 0 to 9.203, 0 and previous response = 2830.                             |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:14:23 AM | Manually integrate compound m+p-Xylenes in sample 07JAN10.D from x, y = 10.020, 0 to 10.062, 0; result = 93                                                                                                                               |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:14:26 AM | Manually integrate qualifier 91.0 of compound m+p-Xylenes in sample 07JAN10.D from x, y = 10.009, 0 to 10.078, 0; result = 397                                                                                                            |        |         | ✓       |           |
| CmdZeroOutPeak                    | BL2000\mchavez | 1/12/2022 9:14:30 AM | Zero out primary peak of compound m+p-Xylenes in sample 07JAN10.D                                                                                                                                                                         |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/12/2022 9:15:43 AM | Set UserDefined = Qualifier ratio did not meet method criteria for Chloroform, Bromodichloromethane, m+p Xylenes for sample 07JAN10.D; previous value = Qualifier ratio did not meet method criteria for Chloroform, Bromodichloromethane |        |         | ✓       |           |

# Audit Trail report

| Name                              | User           | Time                 | Action                                                                                                                                                                                       | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdSaveBatchTable                 | BL2000\mchavez | 1/12/2022 9:15:57 AM | Save batch<br>D:\Org\Data\VOA5975C\VG010722\QuantResults\VG010722_8260B.batch.bin                                                                                                            |        |         | ✓       |           |
| CmdOpenBatchTable                 | BL2000\mchavez | 1/12/2022 9:29:47 AM | Open batch<br>D:\Org\Data\VOA5975C\VG010722\VG010722_8260B.batch.bin                                                                                                                         |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:30:26 AM | Manually integrate qualifier174.5 of compound Bromoform in sample 07JAN10.D from x, y = 10.594, 0 to 10.661, 0; result = 1221                                                                |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:30:28 AM | Manually integrate qualifier170.5 of compound Bromoform in sample 07JAN10.D from x, y = 10.580, 0 to 10.692, 0; result = 1208                                                                |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/12/2022 9:30:43 AM | Set SampleApproved = True for sample 07JAN10.D; previous value = False                                                                                                                       |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:31:16 AM | Manually integrate compound o-Xylene in sample 07JAN11.D from x, y = 10.405, 0 to 10.466, 0; result = 64                                                                                     |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:31:17 AM | Manually integrate qualifier91.0 of compound o-Xylene in sample 07JAN11.D from x, y = 10.416, 0 to 10.458, 0; result = 44                                                                    |        |         | ✓       |           |
| CmdZeroOutPeak                    | BL2000\mchavez | 1/12/2022 9:31:20 AM | Zero out primary peak of compound o-Xylene in sample 07JAN11.D                                                                                                                               |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:31:30 AM | Manually integrate compound m+p-Xylenes in sample 07JAN11.D from x, y = 10.028, 0 to 10.056, 0; result = 316                                                                                 |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:31:34 AM | Manually integrate qualifier91.0 of compound m+p-Xylenes in sample 07JAN11.D from x, y = 10.031, 0 to 10.062, 0; result = 279                                                                |        |         | ✓       |           |
| CmdZeroOutPeak                    | BL2000\mchavez | 1/12/2022 9:31:37 AM | Zero out primary peak of compound m+p-Xylenes in sample 07JAN11.D                                                                                                                            |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/12/2022 9:31:47 AM | Set UserDefined = Qualifier ratio did not meet method criteria for m+p Xylenes for sample 07JAN11.D; previous value =                                                                        |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/12/2022 9:32:00 AM | Set UserDefined = Qualifier ratio did not meet method criteria for m+p Xylenes, o-Xylene for sample 07JAN11.D; previous value = Qualifier ratio did not meet method criteria for m+p Xylenes |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:32:23 AM | Manually integrate compound 1,3-Dichloropropane in sample 07JAN11.D from x, y = 8.946, 0 to 9.022, 0; result = 319                                                                           |        |         | ✓       |           |

# Audit Trail report

| Name                              | User           | Time                 | Action                                                                                                                                                                                                                        | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:32:25 AM | Manually integrate qualifier78.0 of compound 1,3-Dichloropropane in sample 07JAN11.D from x, y = 8.946, 0 to 9.005, 0; result = 72                                                                                            |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/12/2022 9:32:28 AM | Set UserAnnotation = NI for compound 1,3-Dichloropropane in sample 07JAN11.D; previous value =                                                                                                                                |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:32:37 AM | Manually integrate compound 1,1,2-Trichloroethane in sample 07JAN11.D from x, y = 8.776, 0 to 8.854, 0; result = 383                                                                                                          |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:32:39 AM | Manually integrate qualifier97.0 of compound 1,1,2-Trichloroethane in sample 07JAN11.D from x, y = 8.782, 0 to 8.865, 0; result = 527                                                                                         |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:32:43 AM | Manually integrate qualifier85.0 of compound 1,1,2-Trichloroethane in sample 07JAN11.D from x, y = 8.787, 0 to 8.854, 0; result = 86                                                                                          |        |         | ✓       |           |
| CmdZeroOutPeak                    | BL2000\mchavez | 1/12/2022 9:32:47 AM | Zero out primary peak of compound 1,1,2-Trichloroethane in sample 07JAN11.D                                                                                                                                                   |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/12/2022 9:33:16 AM | Set UserDefined = Qualifier ratio did not meet method criteria for m+p Xylenes, o-Xylene, 1,1,2-Trichloroethane for sample 07JAN11.D; previous value = Qualifier ratio did not meet method criteria for m+p Xylenes, o-Xylene |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:33:28 AM | Manually integrate compound Toluene in sample 07JAN11.D from x, y = 8.361, 0 to 8.430, 0; result = 699                                                                                                                        |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:33:30 AM | Manually integrate qualifier91.0 of compound Toluene in sample 07JAN11.D from x, y = 8.349, 0 to 8.433, 0; result = 1384                                                                                                      |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/12/2022 9:33:36 AM | Set UserAnnotation = NI for compound Toluene in sample 07JAN11.D; previous value =                                                                                                                                            |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:35:15 AM | Manually integrate compound Benzene in sample 07JAN11.D from x, y = 6.205, 0 to 6.333, 0; result = 1404                                                                                                                       |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:35:16 AM | Manually integrate qualifier77.0 of compound Benzene in sample 07JAN11.D from x, y = 6.250, 0 to 6.314, 0; result = 156                                                                                                       |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/12/2022 9:35:20 AM | Set UserAnnotation = NI for compound Benzene in sample 07JAN11.D; previous value =                                                                                                                                            |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:35:40 AM | Manually integrate compound Chloroform in sample 07JAN11.D from x, y = 5.614, 0 to 5.711, -70; result = 983                                                                                                                   |        |         | ✓       |           |

# Audit Trail report

| Name                              | User           | Time                 | Action                                                                                                                                                                                              | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:35:45 AM | Manually integrate compound Chloroform in sample 07JAN11.D, from x, y = 5.614, 0 to 5.689, 0, result = 777; previous integration is from x, y = 5.614, 0 to 5.711, -70 and previous response = 983. |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:35:47 AM | Manually integrate qualifier85.0 of compound Chloroform in sample 07JAN11.D from x, y = 5.628, 0 to 5.700, 0; result = 368                                                                          |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/12/2022 9:35:49 AM | Set UserAnnotation = NI for compound Chloroform in sample 07JAN11.D; previous value =                                                                                                               |        |         | ✓       |           |



# Audit Trail report

| Name                     | User           | Time                 | Action                                                                                                          | Reason | Comment | Succeed | Exception                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           |
|--------------------------|----------------|----------------------|-----------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/12/2022 9:36:02 AM | Manually integrate compound 1,1-Dichloroethane in sample 07JAN11.D from x, y = 4.328, 0 to 4.459, 0; result = 0 |        |         |         | Agilent.MassSpectrometry.DataAnalysis.Quantitative.ApplicationCommandException: Manual integration failed for compound 1,1-Dichloroethane in sample B22010219-001F. ---><br>Agilent.MassSpectrometry.DataAnalysis.Quantitative.ApplicationCommandException: Manual integration failed for compound 1,1-Dichloroethane in sample B22010219-001F. ---><br>System.IndexOutOfRangeException: Index was outside the bounds of the array.<br>at<br>at Agilent.MassSpectrometry.DataAnalysis.AgileIntegrator.Peak.a(Double[] A_0, Single[] A_1, Int32 A_2, Int32 A_3, Int32 A_4, Double A_5, Double A_6, Double& A_7, Double& A_8, Int32& A_9, Int32& A_10, Int32& A_11, Int32& A_12)<br>at<br>at Agilent.MassSpectrometry.DataAnalysis.AgileIntegrator.Peak.ComputeChromatographicMetrics(Double[] xArray, Single[] yArray, Int32 startIndex, Int32 apexIndex, Int32 endIndex, Double baselineSlope, Double yIntercept, Double& fullWidthHalfMaximum, Double& symmetry)<br>at<br>at Agilent.MassSpectrometry.DataAnalysis.Quantitative.Integrator.a(IChromatogram A_0, IPeakList A_1)<br>at<br>at Agilent.MassSpectrometry.DataAnalysis.Quantitative.Integrator.ManualIntegrate(IChromatogram chromatogram, Double xStart, Double yStart, Double xEnd, Double yEnd, IChromPeakList& peaklist)<br>at<br>at Agilent.MassSpectrometry.DataAnalysis.Quantitative.Analysis.MeasuredIon.ManualIntegrate(Double xStart, Double yStart, Double xEnd, Double yEnd)<br>--- End of inner exception stack trace ---<br>at<br>at Agilent.MassSpectrometry.DataAnalysis.Quantitative.Analysis.QuantifierIon.SetManualIntegrationFailureMessage(Exception e)<br>at<br>at Agilent.MassSpectrometry.DataAnalysis.Quantitative.Analysis.MeasuredIon.ManualIntegrate(Double xStart, Double yStart, Double xEnd, Double yEnd) |

# Audit Trail report

| Name | User | Time | Action | Reason | Comment | Succeed | Exception                                                                                                                                                                                                                                                                                                                                                                                                                |
|------|------|------|--------|--------|---------|---------|--------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
|      |      |      |        |        |         |         | at<br>Agilent.MassSpectrometry.DataAnalysis.Quantitative.CmdManuallyIntegratePeak.Do()<br>--- End of inner exception stack<br>trace ---<br>at<br>Agilent.MassSpectrometry.DataAnalysis.Quantitative.CmdManuallyIntegratePeak.Do()<br>at<br>Agilent.MassSpectrometry.CommandModel.CommandHistory.Invoke(ICommand cmd)<br>at<br>Agilent.MassSpectrometry.DataAnalysis.Quantitative.AppCommandContext._Invoke(ICommand cmd) |

# Audit Trail report

| Name                                  | User           | Time                 | Action                                                                                                                            | Reason | Comment | Succeed | Exception                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                          |
|---------------------------------------|----------------|----------------------|-----------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| CmdManuallyIntegrate<br>QualifierPeak | BL2000\mchavez | 1/12/2022 9:36:06 AM | Manually integrate qualifier 65.0 of compound 1,1-Dichloroethane in sample 07JAN11.D from x, y = 4.328, 0 to 4.401, 0; result = 0 |        |         |         | Agilent.MassSpectrometry.DataAnalysis.Quantitative.ApplicationCommandException: Manual integration failed for qualifier 65.0 of compound 1,1-Dichloroethane in sample B22010219-001F. ---><br>Agilent.MassSpectrometry.DataAnalysis.Quantitative.ApplicationCommandException: Manual integration failed for qualifier 65.0 of compound 1,1-Dichloroethane in sample B22010219-001F. ---><br>System.IndexOutOfRangeException: Index was outside the bounds of the array.<br>at<br>Agilent.MassSpectrometry.DataAnalysis.AgileIntegrator.Peak.a(Double[] A_0, Single[] A_1, Int32 A_2, Int32 A_3, Int32 A_4, Double A_5, Double A_6, Double A_7, Double A_8, Int32 A_9, Int32 A_10, Int32 A_11, Int32 A_12)<br>at<br>Agilent.MassSpectrometry.DataAnalysis.AgileIntegrator.Peak.ComputeChromatographicMetrics(Double[] xArray, Single[] yArray, Int32 startIndex, Int32 apexIndex, Int32 endIndex, Double baselineSlope, Double yIntercept, Double fullWidthHalfMaximum, Double symmetry)<br>at<br>Agilent.MassSpectrometry.DataAnalysis.Quantitative.Integrator.a(ICHromatogram A_0, IPeakList A_1)<br>at<br>Agilent.MassSpectrometry.DataAnalysis.Quantitative.Integrator.ManualIntegrate(ICHromatogram chromatogram, Double xStart, Double yStart, Double xEnd, Double yEnd, IChromPeakList peaklist)<br>at<br>Agilent.MassSpectrometry.DataAnalysis.Quantitative.Analysis.MeasuredIon.ManualIntegrate(Double xStart, Double yStart, Double xEnd, Double yEnd)<br>--- End of inner exception stack trace ---<br>at<br>Agilent.MassSpectrometry.DataAnalysis.Quantitative.Analysis.QualifierIon.SetManualIntegrationFailureMessage(Exception e)<br>at<br>Agilent.MassSpectrometry.DataAnalysis.Quantitative.Analysis.MeasuredIon.M |

# Audit Trail report

| Name                              | User           | Time                 | Action                                                                                                                              | Reason | Comment | Succeed | Exception                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                            |
|-----------------------------------|----------------|----------------------|-------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
|                                   |                |                      |                                                                                                                                     |        |         |         | anualIntegrate(Double xStart, Double yStart, Double xEnd, Double yEnd)<br>at<br>Agilent.MassSpectrometry.DataAnalysis.Quantitative.CmdManuallyIntegrateQualifierPeak.Do()<br>--- End of inner exception stack<br>trace ---<br>at<br>Agilent.MassSpectrometry.DataAnalysis.Quantitative.CmdManuallyIntegrateQualifierPeak.Do()<br>at<br>Agilent.MassSpectrometry.CommandModel.CommandHistory.Invoke(ICommand cmd)<br>at<br>Agilent.MassSpectrometry.DataAnalysis.Quantitative.AppCommandContext._Invoke(ICommand cmd) |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:36:10 AM | Manually integrate qualifier83.0 of compound 1,1-Dichloroethane in sample 07JAN11.D from x, y = 4.348, 0 to 4.445, 0; result = 0    |        |         | ✓       |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                      |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:36:13 AM | Manually integrate compound 1,1-Dichloroethane in sample 07JAN11.D from x, y = 4.339, 0 to 4.448, 0; result = 953                   |        |         | ✓       |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                      |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:36:16 AM | Manually integrate qualifier65.0 of compound 1,1-Dichloroethane in sample 07JAN11.D from x, y = 4.320, 0 to 4.412, 0; result = 177  |        |         | ✓       |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                      |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/12/2022 9:36:19 AM | Set UserAnnotation = NI for compound 1,1-Dichloroethane in sample 07JAN11.D; previous value =                                       |        |         | ✓       |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                      |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:37:13 AM | Manually integrate compound Methylene chloride in sample 07JAN11.D from x, y = 3.291, 0 to 3.394, 0; result = 1285                  |        |         | ✓       |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                      |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:37:15 AM | Manually integrate qualifier84.0 of compound Methylene chloride in sample 07JAN11.D from x, y = 3.296, 0 to 3.377, 0; result = 1048 |        |         | ✓       |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                      |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:37:18 AM | Manually integrate qualifier86.0 of compound Methylene chloride in sample 07JAN11.D from x, y = 3.299, 0 to 3.394, 0; result = 702  |        |         | ✓       |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                      |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/12/2022 9:37:20 AM | Set UserAnnotation = NI for compound Methylene chloride in sample 07JAN11.D; previous value =                                       |        |         | ✓       |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                      |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:37:32 AM | Manually integrate compound Chloroethane in sample 07JAN11.D from x, y = 1.869, 0 to 1.922, 0; result = 1604                        |        |         | ✓       |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                      |

# Audit Trail report

| Name                              | User           | Time                 | Action                                                                                                                              | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|-------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:37:35 AM | Manually integrate qualifier66.0 of compound Chloroethane in sample 07JAN11.D from x, y = 1.869, 0 to 1.911, -2; result = 433       |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/12/2022 9:37:37 AM | Set UserAnnotation = NI for compound Chloroethane in sample 07JAN11.D; previous value =                                             |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:37:48 AM | Manually integrate compound Chloromethane in sample 07JAN11.D from x, y = 1.381, 0 to 1.456, 0; result = 1302                       |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/12/2022 9:37:51 AM | Set UserAnnotation = NI for compound Chloromethane in sample 07JAN11.D; previous value =                                            |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:37:53 AM | Manually integrate qualifier52.0 of compound Chloromethane in sample 07JAN11.D from x, y = 1.378, 0 to 1.459, 0; result = 301       |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/12/2022 9:37:58 AM | Set SampleApproved = True for sample 07JAN11.D; previous value = False                                                              |        |         | ✓       |           |
| CmdQuantitate                     | BL2000\mchavez | 1/12/2022 9:38:16 AM | Quantitate all compounds in all samples                                                                                             |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:38:53 AM | Manually integrate compound Chloromethane in sample 07JAN12.D from x, y = 1.372, 0 to 1.442, 0; result = 854                        |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:38:56 AM | Manually integrate qualifier52.0 of compound Chloromethane in sample 07JAN12.D from x, y = 1.403, 0 to 1.450, 0; result = 97        |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/12/2022 9:38:59 AM | Set UserAnnotation = NI for compound Chloromethane in sample 07JAN12.D; previous value =                                            |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:39:27 AM | Manually integrate compound Methyl ethyl ketone in sample 07JAN12.D from x, y = 5.265, 0 to 5.352, 0; result = 565                  |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:39:30 AM | Manually integrate qualifier72.0 of compound Methyl ethyl ketone in sample 07JAN12.D from x, y = 5.254, 0 to 5.352, 0; result = 130 |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:39:43 AM | Manually integrate compound Chloroform in sample 07JAN12.D from x, y = 5.608, 0 to 5.706, 0; result = 1655                          |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:39:46 AM | Manually integrate qualifier85.0 of compound Chloroform in sample 07JAN12.D from x, y = 5.608, 0 to 5.714, 0; result = 947          |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:40:08 AM | Manually integrate compound Benzene in sample 07JAN12.D from x, y = 6.252, 0 to 6.314, 0; result = 409                              |        |         | ✓       |           |

# Audit Trail report

| Name                              | User           | Time                 | Action                                                                                                                                                                                                                                | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:40:11 AM | Manually integrate qualifier 65.0 of compound 1,2-Dichloroethane-d4 in sample 07JAN12.D, from x, y = 6.261, 0 to 6.275, 2250, result = 3576; previous integration is from x, y = 6.188, 0 to 6.316, 0 and previous response = 182216. |        |         | ✓       |           |
| CmdClearManualIntegration         | BL2000\mchavez | 1/12/2022 9:40:16 AM | Clear manual integration of qualifier 65.0 for compound 1,2-Dichloroethane-d4 in sample 07JAN12.D                                                                                                                                     |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:40:23 AM | Manually integrate qualifier 77.0 of compound Benzene in sample 07JAN12.D from x, y = 6.244, 0 to 6.305, 0; result = 43                                                                                                               |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:40:34 AM | Manually integrate compound Dibromomethane in sample 07JAN12.D from x, y = 7.373, 0 to 7.426, 0; result = 111                                                                                                                         |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:40:36 AM | Manually integrate qualifier 95.0 of compound Dibromomethane in sample 07JAN12.D from x, y = 7.376, 0 to 7.429, 0; result = 67                                                                                                        |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:40:38 AM | Manually integrate qualifier 173.5 of compound Dibromomethane in sample 07JAN12.D from x, y = 7.373, 0 to 7.437, 0; result = 135                                                                                                      |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/12/2022 9:40:40 AM | Set UserAnnotation = NI for compound Dibromomethane in sample 07JAN12.D; previous value =                                                                                                                                             |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/12/2022 9:40:44 AM | Set UserAnnotation = NI for compound Benzene in sample 07JAN12.D; previous value =                                                                                                                                                    |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/12/2022 9:40:47 AM | Set UserAnnotation = NI for compound Methyl ethyl ketone in sample 07JAN12.D; previous value =                                                                                                                                        |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/12/2022 9:40:51 AM | Set UserAnnotation = NI for compound Chloroform in sample 07JAN12.D; previous value =                                                                                                                                                 |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:40:57 AM | Manually integrate compound Bromodichloromethane in sample 07JAN12.D from x, y = 7.557, 0 to 7.624, 0; result = 654                                                                                                                   |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:40:59 AM | Manually integrate qualifier 85.0 of compound Bromodichloromethane in sample 07JAN12.D from x, y = 7.543, 0 to 7.633, 0; result = 391                                                                                                 |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:41:01 AM | Manually integrate qualifier 127.0 of compound Bromodichloromethane in sample 07JAN12.D from x, y = 7.552, 0 to 7.608, 0; result = 34                                                                                                 |        |         | ✓       |           |

# Audit Trail report

| Name                          | User           | Time                 | Action                                                                                                 | Reason | Comment | Succeed | Exception |
|-------------------------------|----------------|----------------------|--------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/12/2022 9:41:10 AM | Set UserAnnotation = NI for compound Bromodichloromethane in sample 07JAN12.D; previous value =        |        |         | ✓       |           |
| CmdManuallyIntegratePeak      | BL2000\mchavez | 1/12/2022 9:41:22 AM | Manually integrate compound Toluene in sample 07JAN12.D from x, y = 8.369, 0 to 8.422, 0; result = 493 |        |         | ✓       |           |

# Audit Trail report

| Name                                  | User           | Time                 | Action                                                                                                                 | Reason | Comment | Succeed | Exception                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                   |
|---------------------------------------|----------------|----------------------|------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| CmdManuallyIntegrate<br>QualifierPeak | BL2000\mchavez | 1/12/2022 9:41:25 AM | Manually integrate qualifier 91.0 of compound Toluene in sample 07JAN12.D from x, y = 8.338, 0 to 8.436, 0; result = 0 |        |         |         | <p>Agilent.MassSpectrometry.DataAnalysis.Quantitative.ApplicationCommandException: Manual integration failed for qualifier 91.0 of compound Toluene in sample B22010213-002C. ---&gt;</p> <p>Agilent.MassSpectrometry.DataAnalysis.Quantitative.ApplicationCommandException: Manual integration failed for qualifier 91.0 of compound Toluene in sample B22010213-002C. ---&gt;</p> <p>System.IndexOutOfRangeException: Index was outside the bounds of the array.</p> <p>at<br/>Agilent.MassSpectrometry.DataAnalysis.AgileIntegrator.Peak.a(Double[] A_0, Single[] A_1, Int32 A_2, Int32 A_3, Int32 A_4, Double A_5, Double A_6, Double&amp; A_7, Double&amp; A_8, Int32&amp; A_9, Int32&amp; A_10, Int32&amp; A_11, Int32&amp; A_12)</p> <p>at<br/>Agilent.MassSpectrometry.DataAnalysis.AgileIntegrator.Peak.ComputeChromatographicMetrics(Double[] xArray, Single[] yArray, Int32 startIndex, Int32 apexIndex, Int32 endIndex, Double baselineSlope, Double yIntercept, Double&amp; fullWidthHalfMaximum, Double&amp; symmetry)</p> <p>at<br/>Agilent.MassSpectrometry.DataAnalysis.Quantitative.Integrator.a(IChromatogram A_0, IPeakList A_1)</p> <p>at<br/>Agilent.MassSpectrometry.DataAnalysis.Quantitative.Integrator.ManualIntegrate(IChromatogram chromatogram, Double xStart, Double yStart, Double xEnd, Double yEnd, IChromPeakList&amp; peaklist)</p> <p>at<br/>Agilent.MassSpectrometry.DataAnalysis.Quantitative.Analysis.MeasuredIon.ManualIntegrate(Double xStart, Double yStart, Double xEnd, Double yEnd)</p> <p>--- End of inner exception stack trace ---</p> <p>at<br/>Agilent.MassSpectrometry.DataAnalysis.Quantitative.Analysis.QualifierIon.SetManualIntegrationFailureMessage(Exception e)</p> <p>at<br/>Agilent.MassSpectrometry.DataAnalysis.Quantitative.Analysis.MeasuredIon.ManualIntegrate(Double xStart, Double yStart, Double xEnd, Double yEnd)</p> |



# Audit Trail report

| Name                              | User           | Time                 | Action                                                                                                                                                                                                  | Reason | Comment | Succeed | Exception                                                                                                                                                                                                                                                                                                                                                                                                                                 |
|-----------------------------------|----------------|----------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
|                                   |                |                      |                                                                                                                                                                                                         |        |         |         | at<br>Agilent.MassSpectrometry.DataAnalysis.Quantitative.CmdManuallyIntegrateQualifierPeak.Do()<br>--- End of inner exception stack<br>trace ---<br>at<br>Agilent.MassSpectrometry.DataAnalysis.Quantitative.CmdManuallyIntegrateQualifierPeak.Do()<br>at<br>Agilent.MassSpectrometry.CommandModel.CommandHistory.Invoke(ICommand cmd)<br>at<br>Agilent.MassSpectrometry.DataAnalysis.Quantitative.AppCommandContext.Invoke(ICommand cmd) |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:41:29 AM | Manually integrate qualifier91.0 of compound Toluene in sample 07JAN12.D from x, y = 8.352, 0 to 8.427, 0; result = 888                                                                                 |        |         | ✓       |                                                                                                                                                                                                                                                                                                                                                                                                                                           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/12/2022 9:41:32 AM | Set UserAnnotation = NI for compound Toluene in sample 07JAN12.D; previous value =                                                                                                                      |        |         | ✓       |                                                                                                                                                                                                                                                                                                                                                                                                                                           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:41:48 AM | Manually integrate compound Chlorodibromomethane in sample 07JAN12.D from x, y = 9.169, 0 to 9.239, 0; result = 1602                                                                                    |        |         | ✓       |                                                                                                                                                                                                                                                                                                                                                                                                                                           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/12/2022 9:41:50 AM | Set UserAnnotation = NI for compound Chlorodibromomethane in sample 07JAN12.D; previous value =                                                                                                         |        |         | ✓       |                                                                                                                                                                                                                                                                                                                                                                                                                                           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:41:52 AM | Manually integrate qualifier127.0 of compound Chlorodibromomethane in sample 07JAN12.D from x, y = 9.175, 0 to 9.244, 0; result = 973                                                                   |        |         | ✓       |                                                                                                                                                                                                                                                                                                                                                                                                                                           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:42:09 AM | Manually integrate compound Ethylbenzene in sample 07JAN12.D, from x, y = 9.875, 0 to 9.944, 0, result = 1441; previous integration is from x, y = 10.009, 0 to 10.059, 0 and previous response = 3201. |        |         | ✓       |                                                                                                                                                                                                                                                                                                                                                                                                                                           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:42:12 AM | Manually integrate qualifier106.0 of compound Ethylbenzene in sample 07JAN12.D from x, y = 9.908, 0 to 9.958, 0; result = 144                                                                           |        |         | ✓       |                                                                                                                                                                                                                                                                                                                                                                                                                                           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/12/2022 9:42:16 AM | Set UserAnnotation = NI for compound Ethylbenzene in sample 07JAN12.D; previous value =                                                                                                                 |        |         | ✓       |                                                                                                                                                                                                                                                                                                                                                                                                                                           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:42:21 AM | Manually integrate compound m+p-Xylenes in sample 07JAN12.D from x, y = 10.006, 0 to 10.070, 0; result = 1346                                                                                           |        |         | ✓       |                                                                                                                                                                                                                                                                                                                                                                                                                                           |

# Audit Trail report

| Name                              | User           | Time                 | Action                                                                                                                                                                                                                                                          | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:42:32 AM | Manually integrate qualifier 91.0 of compound m+p-Xylenes in sample 07JAN12.D, from x, y = 10.009, 0 to 10.059, 26, result = 3162; previous integration is from x, y = 10.009, 0 to 10.073, 0 and previous response = 3521.                                     |        |         | ✓       |           |
| CmdManuallyIntegrateDropBaseline  | BL2000\mchavez | 1/12/2022 9:42:35 AM | Drop baseline for qualifier 91.0 of compound m+p-Xylenes in sample 07JAN12.D to y = 0, new integration is from x, y = 10.009, 0 to 10.059, 0 and new response = 3201; previous integration is from x, y = 10.009, 0 to 10.059, 26 and previous response = 3162. |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:42:39 AM | Manually integrate qualifier 91.0 of compound m+p-Xylenes in sample 07JAN12.D, from x, y = 10.017, 19 to 10.059, 0, result = 3051; previous integration is from x, y = 10.009, 0 to 10.059, 0 and previous response = 3201.                                     |        |         | ✓       |           |
| CmdManuallyIntegrateDropBaseline  | BL2000\mchavez | 1/12/2022 9:42:41 AM | Drop baseline for qualifier 91.0 of compound m+p-Xylenes in sample 07JAN12.D to y = 0, new integration is from x, y = 10.017, 0 to 10.059, 0 and new response = 3074; previous integration is from x, y = 10.017, 19 to 10.059, 0 and previous response = 3051. |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/12/2022 9:42:48 AM | Set UserAnnotation = NI for compound m+p-Xylenes in sample 07JAN12.D; previous value =                                                                                                                                                                          |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:43:02 AM | Manually integrate qualifier 174.5 of compound Bromoform in sample 07JAN12.D from x, y = 10.586, 0 to 10.681, 0; result = 1218                                                                                                                                  |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:43:04 AM | Manually integrate qualifier 170.5 of compound Bromoform in sample 07JAN12.D from x, y = 10.575, 0 to 10.678, 0; result = 1221                                                                                                                                  |        |         | ✓       |           |
| CmdZeroOutPeak                    | BL2000\mchavez | 1/12/2022 9:43:09 AM | Zero out primary peak of compound 1,1,2,2-Tetrachloroethane in sample 07JAN12.D                                                                                                                                                                                 |        |         | ✓       |           |
| CmdZeroOutPeak                    | BL2000\mchavez | 1/12/2022 9:43:18 AM | Zero out primary peak of compound 1,2,3-Trichloropropane in sample 07JAN12.D                                                                                                                                                                                    |        |         | ✓       |           |
| CmdZeroOutPeak                    | BL2000\mchavez | 1/12/2022 9:43:27 AM | Zero out primary peak of compound 4-Chlorotoluene in sample 07JAN12.D                                                                                                                                                                                           |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/12/2022 9:43:35 AM | Set SampleApproved = True for sample 07JAN12.D; previous value = False                                                                                                                                                                                          |        |         | ✓       |           |
| CmdQuantitate                     | BL2000\mchavez | 1/12/2022 9:43:56 AM | Quantitate all compounds in all samples                                                                                                                                                                                                                         |        |         | ✓       |           |

# Audit Trail report

| Name                                  | User           | Time                 | Action                                                                                                                                 | Reason | Comment | Succeed | Exception |
|---------------------------------------|----------------|----------------------|----------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdManuallyIntegrate<br>QualifierPeak | BL2000\mchavez | 1/12/2022 9:45:41 AM | Manually integrate qualifier52.0 of<br>compound Chloromethane in sample<br>07JAN14.D from x, y = 1.372, 0 to<br>1.436, 0; result = 725 |        |         | ✓       |           |

# Audit Trail report

| Name                     | User           | Time                 | Action                                                                                               | Reason | Comment | Succeed | Exception                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                |
|--------------------------|----------------|----------------------|------------------------------------------------------------------------------------------------------|--------|---------|---------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| CmdManuallyIntegratePeak | BL2000\mchavez | 1/12/2022 9:46:20 AM | Manually integrate compound Toluene in sample 07JAN14.D from x, y = 8.338, 0 to 8.444, 0; result = 0 |        |         |         | Agilent.MassSpectrometry.DataAnalysis.Quantitative.ApplicationCommandException: Manual integration failed for compound Toluene in sample B22010214-001F. ---><br>Agilent.MassSpectrometry.DataAnalysis.Quantitative.ApplicationCommandException: Manual integration failed for compound Toluene in sample B22010214-001F. ---><br>System.IndexOutOfRangeException: Index was outside the bounds of the array.<br>at<br>Agilent.MassSpectrometry.DataAnalysis.AgileIntegrator.Peak.a(Double[] A_0, Single[] A_1, Int32 A_2, Int32 A_3, Int32 A_4, Double A_5, Double A_6, Double& A_7, Double& A_8, Int32& A_9, Int32& A_10, Int32& A_11, Int32& A_12)<br>at<br>Agilent.MassSpectrometry.DataAnalysis.AgileIntegrator.Peak.ComputeChromatographicMetrics(Double[] xArray, Single[] yArray, Int32 startIndex, Int32 apexIndex, Int32 endIndex, Double baselineSlope, Double yIntercept, Double& fullWidthHalfMaximum, Double& symmetry)<br>at<br>Agilent.MassSpectrometry.DataAnalysis.Quantitative.Integrator.a(IChromatogram A_0, IPeakList A_1)<br>at<br>Agilent.MassSpectrometry.DataAnalysis.Quantitative.Integrator.ManualIntegrate(IChromatogram chromatogram, Double xStart, Double yStart, Double xEnd, Double yEnd, IChromPeakList& peaklist)<br>at<br>Agilent.MassSpectrometry.DataAnalysis.Quantitative.Analysis.MeasuredIon.ManualIntegrate(Double xStart, Double yStart, Double xEnd, Double yEnd)<br>--- End of inner exception stack trace ---<br>at<br>Agilent.MassSpectrometry.DataAnalysis.Quantitative.Analysis.QuantifierIon.SetManualIntegrationFailureMessage(Exception e)<br>at<br>Agilent.MassSpectrometry.DataAnalysis.Quantitative.Analysis.MeasuredIon.ManualIntegrate(Double xStart, Double yStart, Double xEnd, Double yEnd) |

# Audit Trail report

| Name                              | User           | Time                 | Action                                                                                                                 | Reason | Comment | Succeed | Exception                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                     |
|-----------------------------------|----------------|----------------------|------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
|                                   |                |                      |                                                                                                                        |        |         |         | at<br>Agilent.MassSpectrometry.DataAnalysis.Quantitative.CmdManuallyIntegratePeak.Do()<br>--- End of inner exception stack<br>trace ---<br>at<br>Agilent.MassSpectrometry.DataAnalysis.Quantitative.CmdManuallyIntegratePeak.Do()<br>at<br>Agilent.MassSpectrometry.CommandModel.CommandHistory.Invoke(ICommand cmd)<br>at<br>Agilent.MassSpectrometry.DataAnalysis.Quantitative.AppCommandContext._Invoke(ICommand cmd)                                                                                      |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:46:25 AM | Manually integrate qualifier 91.0 of compound Toluene in sample 07JAN14.D from x, y = 8.341, 0 to 8.419, 0; result = 0 |        |         | ✓       |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                               |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:46:28 AM | Manually integrate compound Toluene in sample 07JAN14.D from x, y = 8.344, 0 to 8.433, 0; result = 667                 |        |         | ✓       |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                               |
| CmdClearManualIntegration         | BL2000\mchavez | 1/12/2022 9:46:49 AM | Clear manual integration of target signal for compound Toluene in sample 07JAN14.D                                     |        |         |         | Agilent.MassSpectrometry.DataAnalysis.Quantitative.ApplicationCommandException: Integrator did not find any peaks<br>at<br>Agilent.MassSpectrometry.DataAnalysis.Quantitative.Analysis.MeasuredIon.ClearManualIntegration()<br>at<br>Agilent.MassSpectrometry.DataAnalysis.Quantitative.CmdClearManualIntegration.Do()<br>at<br>Agilent.MassSpectrometry.CommandModel.CommandHistory.Invoke(ICommand cmd)<br>at<br>Agilent.MassSpectrometry.DataAnalysis.Quantitative.AppCommandContext._Invoke(ICommand cmd) |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:47:15 AM | Manually integrate compound Toluene in sample 07JAN14.D from x, y = 8.355, 0 to 8.436, 0; result = 667                 |        |         | ✓       |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                               |
| CmdZeroOutPeak                    | BL2000\mchavez | 1/12/2022 9:47:17 AM | Zero out primary peak of compound Toluene in sample 07JAN14.D                                                          |        |         | ✓       |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                               |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/12/2022 9:47:40 AM | Set UserDefined = Qualifier ratio did not meet method criteria for Toluene for sample 07JAN14.D; previous value =      |        |         | ✓       |                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                               |

# Audit Trail report

| Name                              | User           | Time                 | Action                                                                                                                                  | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|-----------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:48:16 AM | Manually integrate compound Methylene chloride in sample 07JAN14.D from x, y = 3.302, 0 to 3.400, 0; result = 885                       |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:48:18 AM | Manually integrate qualifier84.0 of compound Methylene chloride in sample 07JAN14.D from x, y = 3.302, 0 to 3.375, 0; result = 448      |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:48:20 AM | Manually integrate qualifier86.0 of compound Methylene chloride in sample 07JAN14.D from x, y = 3.302, 0 to 3.383, 0; result = 313      |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/12/2022 9:48:24 AM | Set UserAnnotation = NI for compound Methylene chloride in sample 07JAN14.D; previous value =                                           |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/12/2022 9:48:49 AM | Set SampleApproved = True for sample 07JAN14.D; previous value = False                                                                  |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:49:15 AM | Manually integrate compound Dichlorodifluoromethane in sample 07JAN15.D from x, y = 1.219, 0 to 1.300, 0; result = 1185                 |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:49:17 AM | Manually integrate qualifier87.0 of compound Dichlorodifluoromethane in sample 07JAN15.D from x, y = 1.202, 0 to 1.280, 0; result = 350 |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/12/2022 9:49:20 AM | Set UserAnnotation = NI for compound Dichlorodifluoromethane in sample 07JAN15.D; previous value =                                      |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:49:24 AM | Manually integrate compound Chloromethane in sample 07JAN15.D from x, y = 1.386, 0 to 1.422, 0; result = 626                            |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:49:27 AM | Manually integrate qualifier52.0 of compound Chloromethane in sample 07JAN15.D from x, y = 1.397, 0 to 1.434, 0; result = 61            |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/12/2022 9:49:32 AM | Set UserAnnotation = NI for compound Chloromethane in sample 07JAN15.D; previous value =                                                |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:49:51 AM | Manually integrate compound Methylene chloride in sample 07JAN15.D from x, y = 3.299, 0 to 3.372, 0; result = 648                       |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:49:54 AM | Manually integrate qualifier84.0 of compound Methylene chloride in sample 07JAN15.D from x, y = 3.280, 0 to 3.405, 0; result = 450      |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:49:56 AM | Manually integrate qualifier86.0 of compound Methylene chloride in sample 07JAN15.D from x, y = 3.291, 0 to 3.383, 0; result = 284      |        |         | ✓       |           |

# Audit Trail report

| Name                              | User           | Time                 | Action                                                                                                                                                                      | Reason | Comment | Succeed | Exception |
|-----------------------------------|----------------|----------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdSetTargetCompoundAttribute     | BL2000\mchavez | 1/12/2022 9:49:58 AM | Set UserAnnotation = NI for compound Methylene chloride in sample 07JAN15.D; previous value =                                                                               |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:50:12 AM | Manually integrate compound Chloroform in sample 07JAN15.D from x, y = 5.605, 0 to 5.697, 0; result = 600                                                                   |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:50:14 AM | Manually integrate qualifier 85.0 of compound Chloroform in sample 07JAN15.D from x, y = 5.636, 0 to 5.695, 0; result = 88                                                  |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:50:22 AM | Manually integrate compound Benzene in sample 07JAN15.D from x, y = 6.230, 0 to 6.328, 0; result = 748                                                                      |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:50:24 AM | Manually integrate qualifier 77.0 of compound Benzene in sample 07JAN15.D from x, y = 6.238, 0 to 6.314, 0; result = 108                                                    |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:50:39 AM | Manually integrate compound Toluene in sample 07JAN15.D from x, y = 8.355, 0 to 8.430, 0; result = 723                                                                      |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:50:42 AM | Manually integrate qualifier 91.0 of compound Toluene in sample 07JAN15.D from x, y = 8.352, 0 to 8.439, 0; result = 1271                                                   |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:50:59 AM | Manually integrate compound m+p-Xylenes in sample 07JAN15.D from x, y = 9.992, 0 to 10.064, 0; result = 505                                                                 |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:51:01 AM | Manually integrate qualifier 91.0 of compound m+p-Xylenes in sample 07JAN15.D from x, y = 10.009, 0 to 10.064, 0; result = 1116                                             |        |         | ✓       |           |
| CmdManuallyIntegratePeak          | BL2000\mchavez | 1/12/2022 9:51:06 AM | Manually integrate compound o-Xylene in sample 07JAN15.D from x, y = 10.419, 0 to 10.463, 0; result = 172                                                                   |        |         | ✓       |           |
| CmdManuallyIntegrateQualifierPeak | BL2000\mchavez | 1/12/2022 9:51:08 AM | Manually integrate qualifier 91.0 of compound o-Xylene in sample 07JAN15.D from x, y = 10.396, 0 to 10.477, 0; result = 450                                                 |        |         | ✓       |           |
| CmdZeroOutPeak                    | BL2000\mchavez | 1/12/2022 9:51:13 AM | Zero out primary peak of compound o-Xylene in sample 07JAN15.D                                                                                                              |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/12/2022 9:51:25 AM | Set UserDefined = Qualifier ratio did not meet method criteria for Toluene for sample 07JAN15.D; previous value =                                                           |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/12/2022 9:51:35 AM | Set UserDefined = Qualifier ratio did not meet method criteria for o-Xylene for sample 07JAN15.D; previous value = Qualifier ratio did not meet method criteria for Toluene |        |         | ✓       |           |
| CmdSetSampleAttribute             | BL2000\mchavez | 1/12/2022 9:51:44 AM | Set SampleName = B22010262-002A for sample 07JAN09.D; previous value = B22010226-002A                                                                                       |        |         | ✓       |           |

# Audit Trail report

| Name                          | User           | Time                  | Action                                                                                                                                                                                            | Reason | Comment | Succeed | Exception |
|-------------------------------|----------------|-----------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdSetSampleAttribute         | BL2000\mchavez | 1/12/2022 9:52:03 AM  | Set UserDefined = Corrected sample ID from vial run on autosampler. for sample 07JAN09.D; previous value =                                                                                        |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 1/12/2022 9:52:16 AM  | Set UserAnnotation = NI for compound m+p-Xylenes in sample 07JAN15.D; previous value =                                                                                                            |        |         | ✓       |           |
| CmdSetSampleAttribute         | BL2000\mchavez | 1/12/2022 9:52:52 AM  | Set SampleApproved = True for sample 07JAN15.D; previous value = False                                                                                                                            |        |         | ✓       |           |
| CmdQuantitate                 | BL2000\mchavez | 1/12/2022 9:53:07 AM  | Quantitate all compounds in all samples                                                                                                                                                           |        |         | ✓       |           |
| CmdSetSampleAttribute         | BL2000\mchavez | 1/12/2022 9:55:03 AM  | Set SampleApproved = True for sample 07JAN17.D; previous value = False                                                                                                                            |        |         | ✓       |           |
| CmdQuantitate                 | BL2000\mchavez | 1/12/2022 9:55:20 AM  | Quantitate all compounds in all samples                                                                                                                                                           |        |         | ✓       |           |
| CmdSetSampleAttribute         | BL2000\mchavez | 1/12/2022 9:59:39 AM  | Set SampleApproved = True for sample 07JAN18.D; previous value = False                                                                                                                            |        |         | ✓       |           |
| CmdSetSampleAttribute         | BL2000\mchavez | 1/12/2022 10:01:17 AM | Set SampleApproved = True for sample 07JAN20.D; previous value = False                                                                                                                            |        |         | ✓       |           |
| CmdSaveBatchTable             | BL2000\mchavez | 1/12/2022 10:01:26 AM | Save batch<br>D:\Org\Data\VOA5975C\VG010722\QuantResults\VG010722_8260B.batch.bin                                                                                                                 |        |         | ✓       |           |
| CmdOpenBatchTable             | BL2000\mchavez | 3/2/2022 10:30:43 AM  | Open batch<br>D:\Org\Data\VOA5975C\VG010722\VG010722_8260B.batch.bin                                                                                                                              |        |         | ✓       |           |
| CmdSetSampleAttribute         | BL2000\mchavez | 3/2/2022 10:31:09 AM  | Set SampleType = MatrixBlank for sample 07JAN11.D; previous value = Sample                                                                                                                        |        |         | ✓       |           |
| CmdSetSampleAttribute         | BL2000\mchavez | 3/2/2022 10:31:15 AM  | Set SampleApproved = True for sample 07JAN02.D; previous value = False                                                                                                                            |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 3/2/2022 10:31:59 AM  | Set UserAnnotation = LT for compound Chlorodibromomethane in sample 07JAN10.D; previous value =                                                                                                   |        |         | ✓       |           |
| CmdZeroOutPeak                | BL2000\mchavez | 3/2/2022 10:33:29 AM  | Zero out primary peak of compound Chloroform in sample 07JAN15.D                                                                                                                                  |        |         | ✓       |           |
| CmdManuallyIntegratePeak      | BL2000\mchavez | 3/2/2022 10:33:57 AM  | Manually integrate compound Chloroform in sample 07JAN15.D, from x, y = 5.653, 0 to 5.689, 0, result = 129; previous integration is from x, y = 5.653, 0 to 5.653, 0 and previous response = 0.   |        |         | ✓       |           |
| CmdManuallyIntegratePeak      | BL2000\mchavez | 3/2/2022 10:34:00 AM  | Manually integrate compound Chloroform in sample 07JAN15.D, from x, y = 5.600, 0 to 5.689, 0, result = 600; previous integration is from x, y = 5.653, 0 to 5.689, 0 and previous response = 129. |        |         | ✓       |           |



# Audit Trail report

| Name                          | User           | Time                 | Action                                                                                | Reason | Comment | Succeed | Exception |
|-------------------------------|----------------|----------------------|---------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 3/2/2022 10:34:14 AM | Set UserAnnotation = NI for compound Chloroform in sample 07JAN15.D; previous value = |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 3/2/2022 10:34:20 AM | Set UserAnnotation = NI for compound Benzene in sample 07JAN15.D; previous value =    |        |         | ✓       |           |
| CmdSetTargetCompoundAttribute | BL2000\mchavez | 3/2/2022 10:34:23 AM | Set UserAnnotation = NI for compound Toluene in sample 07JAN15.D; previous value =    |        |         | ✓       |           |

# Audit Trail report

| Name         | User           | Time                 | Action                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                   | Reason | Comment | Succeed | Exception |
|--------------|----------------|----------------------|------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdCalibrate | BL2000\mchavez | 3/2/2022 10:36:54 AM | Replace level QC with QC sample 07JAN04.D for compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, o-Xylene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, 1,2-Dichloroethane, Benzene, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1-Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Chloroethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, Toluene};<br>Replace level CC with CC sample 07JAN03.D for compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, o-Xylene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, 1,2-Dichloroethane, Benzene, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1- |        |         | ✓       |           |

# Audit Trail report

| Name              | User           | Time                 | Action                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                            | Reason | Comment | Succeed | Exception |
|-------------------|----------------|----------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
|                   |                |                      | Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Chloroethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, Toluene};                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                    |        |         |         |           |
| CmdQuantitate     | BL2000\mchavez | 3/2/2022 10:37:16 AM | Quantitate all compounds in all samples                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           |        |         | ✓       |           |
| CmdSaveBatchTable | BL2000\mchavez | 3/2/2022 10:40:15 AM | Save batch<br>D:\Org\Data\VOA5975C\VG010722\QuantResults\VG010722_8260B.batch.bin                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                 |        |         | ✓       |           |
| GenerateReport    | BL2000\mchavez | 3/2/2022 10:41:04 AM | Generates report - Method: \\MASSHUNTER\Org\reports\LevelIV_Reports\SampleSequence\CC_mid_rpt.m, Output Path: D:\Org\Data\VOA5975C\VG010722\QuantReports\VG010722_8260B                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                                           |        |         | ✓       |           |
| CmdCalibrate      | BL2000\mchavez | 3/2/2022 10:41:44 AM | Replace level CC with CC sample 07JAN20.D for compounds {1,2-Dichlorobenzene, 1,4-Dichlorobenzene, 1,3-Dichlorobenzene, 4-Chlorotoluene, 2-Chlorotoluene, 1,2,3-Trichloropropane, 1,1,2,2-Tetrachloroethane, Bromobenzene, p-Bromofluorobenzene, Bromoform, Styrene, o-Xylene, m+p-Xylenes, Ethylbenzene, 1,1,1,2-Tetrachloroethane, Chlorobenzene, 1,2-Dibromoethane, Chlorodibromomethane, 1,3-Dichloropropane, Tetrachloroethene, 1,1,2-Trichloroethane, trans-1,3-Dichloropropene, Toluene-d8, cis-1,3-Dichloropropene, Bromodichloromethane, Dibromomethane, 1,2-Dichloropropane, Trichloroethene, 1,2-Dichloroethane, Benzene, 1,2-Dichloroethane-d4, 1,1-Dichloropropene, Carbon tetrachloride, Dibromofluoromethane, 1,1,1-Trichloroethane, Chloroform, Bromochloromethane, Methyl ethyl ketone, cis-1,2-Dichloroethene, 2,2-Dichloropropane, 1,1-Dichloroethane, Methyl tert-butyl ether (MTBE), trans-1,2-Dichloroethene, Methylene chloride, 1,1-Dichloroethene, Trichlorofluoromethane, Chloroethane, Bromomethane, Vinyl chloride, Chloromethane, Dichlorodifluoromethane, Toluene}; |        |         | ✓       |           |

# Audit Trail report

| Name              | User           | Time                 | Action                                                                                                                                                                          | Reason | Comment | Succeed | Exception |
|-------------------|----------------|----------------------|---------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|--------|---------|---------|-----------|
| CmdQuantitate     | BL2000\mchavez | 3/2/2022 10:43:26 AM | Quantitate all compounds in all samples                                                                                                                                         |        |         | ✓       |           |
| CmdSaveBatchTable | BL2000\mchavez | 3/2/2022 10:44:13 AM | Save batch<br>D:\Org\Data\VOA5975C\VG010722\QuantResults\VG010722_8260B.batch.bin                                                                                               |        |         | ✓       |           |
| GenerateReport    | BL2000\mchavez | 3/2/2022 10:44:51 AM | Generates report - Method:<br>\\MASSHUNTER\Org\reports\LevelIV_Reports\SampleSequence\CC_mid_rpt.m, Output Path:<br>D:\Org\Data\VOA5975C\VG010722\QuantReports\VG010722_8260B-1 |        |         | ✓       |           |



# Analytical RunID VOA5975C.I\_220104A Standards Traceability Report

**Standard ID:** VOCF0313

**Standard Name:** Liquids

**Prep Date:** 6/23/2020

**Exp Date:** 4/13/2023

**Department:** gcmsvoa

**Vendor:** AccuStd

**Lot Number:** 220041126

**Balance ID:**

**Comments:** Date Prepared is same as Date Received. 2,000 ug/mL. Catalog # M502A-R-10X. Corrected lot number to match Cl. MSC 01/14/2022

**Type:** Primary

**Prep By:** Alethea M. Shaules

**Status:** New

**Final Volume:** 10 mL

| Chemical/Solvent Used                | Bottle No    | Amt | Units | Expires   |
|--------------------------------------|--------------|-----|-------|-----------|
| Volatile Organic Compounds - Liquids | <u>12797</u> | 1   | mL    | 4/13/2023 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0313     | ug/mL      |              |



# Analytical RunID VOA5975C.I\_220104A Standards Traceability Report

**Spike ID:** VOCF0352

**Spike Name:** 2nd Source Liquids

**Prep Date:** 11/23/2020

**Exp Date:** 12/31/2023

**Department:** gcmsvoa

**Vendor:** Agilent

**Lot Number:** 0006570990

**Balance ID:**

**Comments:** Date Prepared is same as Date Received. 2000 ug/mL in MeOH. Catalog # DWM-589N-1.

**Type:** Primary

**Prep By:** Steve Dilts

**Status:** New

**Final Volume:** 10 mL

| Chemical/Solvent Used | Bottle No    | Amt | Units | Expires    |
|-----------------------|--------------|-----|-------|------------|
| VOC Standard          | <u>13292</u> | 1   | mL    | 12/31/2023 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0352     | ug/mL      |              |



# Analytical RunID VOA5975C.I\_220104A Standards Traceability Report

**Spike ID:** VOCF0364

**Spike Name:** Surrogates 2.0 mg/mL

**Type:** Primary

**Prep Date:** 1/6/2021

**Prep By:** Jerran D. Brenden

**Exp Date:** 4/18/2029

**Status:** New

**Department:** gcmsvoa

**Vendor:** AccuStandard

**Final Volume:** 10 mL

**Lot Number:** 219041458

**Balance ID:**

**Comments:** Date Received 01/04/2021. 2.0 mg/mL. Catalog # M-8260A-B-SS-10X

| Chemical/Solvent Used  | Bottle No    | Amt | Units | Expires   |
|------------------------|--------------|-----|-------|-----------|
| Surrogate Standard Mix | <u>13385</u> | 1   | mL    | 4/18/2029 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0364     | ug/mL      |              |



# Analytical RunID VOA5975C.I\_220104A Standards Traceability Report

**Standard ID:** VOCF0373

**Standard Name:** MtBE (Methy tert-Butyl Ether)

**Prep Date:** 2/26/2021

**Exp Date:** 8/31/2022

**Department:** gcmsvoa

**Vendor:** Agilent

**Lot Number:** 0006555762

**Balance ID:**

**Comments:** Date Prepared is same as Date Received. 2000 ug/mL in MeOH. Catalog # STS-440

**Type:** Primary

**Prep By:** Steve Dilts

**Status:** New

**Final Volume:** 5 mL

| Chemical/Solvent Used            | Bottle No | Amt | Units | Expires   |
|----------------------------------|-----------|-----|-------|-----------|
| Methyl tert-Butyl Ether Standard | 13578     | 1   | mL    | 8/31/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0373     | ug/mL      |              |





# Analytical RunID VOA5975C.I\_220104A Standards Traceability Report

**Spike ID:** VOCF0401

**Spike Name:** 2nd Source MtBE

**Prep Date:** 6/7/2021

**Exp Date:** 12/11/2029

**Department:** gcmsvoa

**Vendor:** AccuStandard

**Lot Number:** 220051182

**Balance ID:**

**Comments:** Date Prepared is same as Date Receive. 2,000 ug/mL in MeOH. Catalog # S-078-10X.

**Type:** Primary

**Prep By:** Alethea M. Shaules

**Status:** New

**Final Volume:** 5 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires    |
|-----------------------|-----------|-----|-------|------------|
| MTBE                  | 13920     | 1   | mL    | 12/11/2029 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0401     | ug/mL      |              |



# Analytical RunID VOA5975C.I\_220104A Standards Traceability Report

**Spike ID:** VOCF0417

**Spike Name:** Chem Service Gases

**Type:** Primary

**Prep Date:** 8/3/2021

**Prep By:** Steve Dilts

**Exp Date:** 2/28/2022

**Status:** New

**Department:** gcmsvoa

**Vendor:** Chemservice

**Final Volume:** 5 mL

**Lot Number:** 11882100

**Balance ID:**

**Comments:** Date Prepared is same as Date Received. 2000 ug/mL in MeOH. Catalog # M-VOHC6M5-1ML

| Chemical/Solvent Used                           | Bottle No    | Amt | Units | Expires   |
|-------------------------------------------------|--------------|-----|-------|-----------|
| Volatile Organics High Concentration Mixture #6 | <u>14142</u> | 5   | mL    | 2/28/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0417     | ug/mL      |              |



# Analytical RunID VOA5975C.I\_220104A Standards Traceability Report

**Standard ID:** VOCF0425

**Standard Name:** Internals

**Prep Date:** 9/8/2021

**Exp Date:** 12/31/2022

**Department:** gcmsvoa

**Vendor:** Agilent

**Lot Number:** 0006582580

**Balance ID:**

**Comments:** Date Prepared is same as Date Received. 2,500 ug/mL in MeOH. Catalog # STM-520-1.

**Type:** Primary

**Prep By:** Jerran D. Brenden

**Status:** New

**Final Volume:** 10 mL

| Chemical/Solvent Used | Bottle No    | Amt          | Units | Expires    |
|-----------------------|--------------|--------------|-------|------------|
| Internal Standard     | <u>14251</u> | 1            | mL    | 12/31/2022 |
| Stock Source          | Base Units   | Amount Added |       |            |
| VOCF0425              | ug/mL        |              |       |            |



# Analytical RunID VOA5975C.I\_220104A Standards Traceability Report

**Spike ID:** VOCF0426

**Spike Name:** Surrogates 2.0 mg/mL

**Prep Date:** 9/14/2021

**Exp Date:** 4/18/2029

**Department:** gcmsvoa

**Vendor:** AccuStandard

**Lot Number:** 219041458

**Balance ID:**

**Comments:** Date Received 01/04/2021. 2.0 mg/mL. Catalog # M-8260A-B-SS-10X

**Type:** Primary

**Prep By:** Jerran D. Brenden

**Status:** New

**Final Volume:** 10 mL

| Chemical/Solvent Used  | Bottle No    | Amt | Units | Expires   |
|------------------------|--------------|-----|-------|-----------|
| Surrogate Standard Mix | <u>14269</u> | 1   | mL    | 4/18/2029 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0426     | ug/mL      |              |



# Analytical RunID VOA5975C.I\_220104A Standards Traceability Report

**Standard ID:** VOCF0427

**Standard Name:** Gases

**Prep Date:** 9/17/2021

**Exp Date:** 8/3/2024

**Department:** gcmsvoa

**Vendor:** Absolute

**Lot Number:** 080321

**Balance ID:**

**Comments:** Date Prepared is same as Date Received. 2,000 ug/mL in MeOH. Catalog # 30058.

**Type:** Primary

**Prep By:** Alethea M. Shaules

**Status:** New

**Final Volume:** 10 mL

| Chemical/Solvent Used                      | Bottle No    | Amt | Units | Expires  |
|--------------------------------------------|--------------|-----|-------|----------|
| EPA Method 502-524 - Volatile Gases Mix #1 | <u>14285</u> | 1   | mL    | 8/3/2024 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0427     | ug/mL      |              |



# Analytical RunID VOA5975C.I\_220104A Standards Traceability Report

**Standard ID:** VOCF0434

**Standard Name:** Ketones

**Prep Date:** 10/26/2021

**Exp Date:** 6/30/2023

**Department:** gcmsvoa

**Vendor:** Chem Service

**Lot Number:** 10251200

**Balance ID:**

**Comments:** Date Prepared is same as Date Received. 2,000 ug/mL in 90:10 MeOH:H2O. Catalog # M-TCL-1AN5-5ML.

**Type:** Primary

**Prep By:** Steve Dilts

**Status:** New

**Final Volume:** 5 mL

| Chemical/Solvent Used | Bottle No    | Amt | Units | Expires   |
|-----------------------|--------------|-----|-------|-----------|
| TCL Ketone Mix        | <u>14443</u> | 1   | mL    | 6/30/2023 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0434     | ug/mL      |              |



# Analytical RunID VOA5975C.I\_220104A Standards Traceability Report

**Standard ID:** VOCF0439

**Standard Name:** 2nd Source Ketones

**Prep Date:** 11/30/2021

**Exp Date:** 11/26/2022

**Department:** gcmsvoa

**Vendor:** AccuStandard

**Lot Number:** 221101480

**Balance ID:**

**Comments:** Date Prepared is same as Date Received. 2,000 ug/mL in Methanol. Catalog # CLP-022K-10X.

**Type:** Primary

**Prep By:** Melissa Chavez

**Status:** New

**Final Volume:** 1 mL

| Chemical/Solvent Used | Bottle No    | Amt | Units | Expires    |
|-----------------------|--------------|-----|-------|------------|
| TCL Ketones Mixture   | <u>14567</u> | 2   | mL    | 11/26/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0439     | ug/mL      |              |



# Analytical RunID VOA5975C.I\_220104A Standards Traceability Report

**Standard ID:** VOCF3473

**Standard Name:** Calibration Surrogates

**Prep Date:** 9/14/2021

**Exp Date:** 3/14/2022

**Department:** gcmsvoa

**Vendor:**

**Lot Number:**

**Balance ID:**

**Comments:** Final Concentration 0.2 ug/uL in MeOH

**Type:** Secondary

**Prep By:** Jerran D. Brenden

**Status:** New

**Final Volume:** 5 mL

| Chemical/Solvent Used          | Bottle No    | Amt          | Units | Expires   |
|--------------------------------|--------------|--------------|-------|-----------|
| Methanol, Purge and Trap EA226 | <u>13754</u> | 4.5          | mL    | 3/14/2022 |
| Stock Source                   | Base Units   | Amount Added |       |           |
| VOCF0364                       | ug/mL        | 0.5 mL       |       |           |





# Analytical RunID VOA5975C.I\_220104A Standards Traceability Report

**Spike ID:** VOCF3517

**Spike Name:** Internal Standard / Surrogates (INT/SURR)

**Type:** Secondary

**Prep Date:** 11/10/2021

**Prep By:** Alethea M. Shaules

**Exp Date:** 12/31/2022

**Status:** New

**Department:** gcmsvoa

**Final Volume:** 100 mL

**Vendor:**

**Lot Number:**

**Balance ID:**

**Comments:** Final Concentration 0.05 ug/uL in MeOH.

| Chemical/Solvent Used               | Bottle No    | Amt  | Units | Expires    |
|-------------------------------------|--------------|------|-------|------------|
| Methanol, Purge and Trap - EB199-US | <u>14334</u> | 95.5 | mL    | 12/31/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0425     | ug/mL      | 2 mL         |
| VOCF0426     | ug/mL      | 2.5 mL       |



# Analytical RunID VOA5975C.I\_220104A Standards Traceability Report

**Spike ID:** VOCF3529B

**Spike Name:** 2nd Source MtBE

**Prep Date:** 11/29/2021

**Exp Date:** 1/29/2022

**Department:** gcmsvoa

**Vendor:**

**Lot Number:**

**Balance ID:**

**Comments:** Final Concentration 0.2 ug/uL

**Type:** Secondary

**Prep By:** Alethea M. Shaules

**Status:**

**Final Volume:** 10 mL

| Chemical/Solvent Used               | Bottle No    | Amt | Units | Expires   |
|-------------------------------------|--------------|-----|-------|-----------|
| Methanol, Purge and Trap - EB199-US | <u>14334</u> | 9   | mL    | 1/29/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0401     | ug/mL      | 1 mL         |



# Analytical RunID VOA5975C.I\_220104A Standards Traceability Report

**Standard ID:** VO CF3546A

**Standard Name:** Liquids

**Prep Date:** 12/13/2021

**Exp Date:** 1/13/2022

**Department:** GCMSVOA

**Vendor:**

**Lot Number:**

**Balance ID:**

**Comments:** 1.0 ml/10 ml final volume. Final Concentration 0.2 ug/uL. Corrected comment and analyte list 11/9/2021 sbd

**Type:** Secondary

**Prep By:** Alethea M. Shaules

**Status:**

**Final Volume:** 10 mL

| Chemical/Solvent Used          | Bottle No    | Amt | Units | Expires   |
|--------------------------------|--------------|-----|-------|-----------|
| Methanol, Purge and Trap EA899 | <u>13926</u> | 9   | mL    | 1/13/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0313     | ug/mL      | 1 mL         |



# Analytical RunID VOA5975C.I\_220104A Standards Traceability Report

**Spike ID:** VOCF3549

**Spike Name:** 2nd Source Ketones

**Prep Date:** 12/15/2021

**Exp Date:** 1/15/2022

**Department:** gcmsvoa

**Vendor:** AccuStandard

**Lot Number:** 221101480

**Balance ID:**

**Comments:** Vial opened for use. 2.0 µg/µL

**Type:** Primary

**Prep By:** Melissa Chavez

**Status:**

**Final Volume:** 1 mL

| Chemical/Solvent Used | Bottle No    | Amt | Units | Expires   |
|-----------------------|--------------|-----|-------|-----------|
| TCL Ketones Mixture   | <u>14567</u> | 1   | mL    | 1/15/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0439     | ug/mL      | 1 mL         |



# Analytical RunID VOA5975C.I\_220104A Standards Traceability Report

**Standard ID:** VOCF3550

**Standard Name:** Ketones

**Prep Date:** 12/16/2021

**Exp Date:** 1/16/2022

**Department:** gcmsvoa

**Vendor:** Chem Service

**Lot Number:** 10251200

**Balance ID:**

**Comments:** Vial Opened For Use . 2.0 ug/uL in 90:10 MeOH:H2O.

**Type:** Primary

**Prep By:** Melissa Chavez

**Status:**

**Final Volume:** 1 mL

| Chemical/Solvent Used | Bottle No    | Amt | Units | Expires   |
|-----------------------|--------------|-----|-------|-----------|
| TCL Ketone Mix        | <u>14443</u> | 1   | mL    | 1/16/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0434     | ug/mL      | 1 mL         |



# Analytical RunID VOA5975C.I\_220104A Standards Traceability Report

**Spike ID:** VOCF3558B

**Spike Name:** 2nd Source Liquids

**Type:** Secondary

**Prep Date:** 12/27/2021

**Prep By:** Steve Dilts

**Exp Date:** 2/27/2022

**Status:** Open

**Department:** gcmsvoa

**Vendor:**

**Final Volume:** 10 mL

**Lot Number:**

**Balance ID:**

**Comments:** Final Concentration 0.2ug/uL.

| Chemical/Solvent Used               | Bottle No    | Amt | Units | Expires   |
|-------------------------------------|--------------|-----|-------|-----------|
| Methanol, Purge and Trap - EB199-US | <u>14334</u> | 9   | mL    | 2/27/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0352     | ug/mL      | 1 mL         |



# Analytical RunID VOA5975C.I\_220104A Standards Traceability Report

**Standard ID:** VOCF3559A

**Standard Name:** MtBE

**Prep Date:** 12/27/2021

**Exp Date:** 1/27/2022

**Department:** gcmsvoa

**Vendor:**

**Lot Number:**

**Balance ID:**

**Comments:** Final Concentration 0.2 ug/uL.

**Type:** Secondary

**Prep By:** Melissa Chavez

**Status:**

**Final Volume:** 10 mL

| Chemical/Solvent Used               | Bottle No    | Amt | Units | Expires   |
|-------------------------------------|--------------|-----|-------|-----------|
| Methanol, Purge and Trap - EB199-US | <u>14334</u> | 9   | mL    | 1/27/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0373     | ug/mL      | 1 mL         |



# Analytical RunID VOA5975C.I\_220104A Standards Traceability Report

**Standard ID:** VOCF3562A

**Standard Name:** Gases

**Prep Date:** 1/3/2022

**Exp Date:** 1/10/2022

**Department:** GCMSVOA

**Vendor:**

**Lot Number:**

**Balance ID:**

**Comments:** 1.0 ml/10 ml final volume. Final Concentration 0.2 ug/uL

**Type:** Secondary

**Prep By:** Alethea M. Shaules

**Status:**

**Final Volume:** 10 mL

| Chemical/Solvent Used          | Bottle No    | Amt | Units | Expires   |
|--------------------------------|--------------|-----|-------|-----------|
| Methanol, Purge and Trap EB373 | <u>14519</u> | 9   | mL    | 1/10/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0427     | ug/mL      | 1 mL         |





# Analytical RunID VOA5975C.I\_220104A Standards Traceability Report

**Standard ID:** VOCF3563

**Standard Name:** Internals

**Prep Date:** 1/3/2022

**Exp Date:** 7/3/2022

**Department:** gcmsvoa

**Vendor:**

**Lot Number:**

**Balance ID:**

**Comments:** Final Concentration 0.05 ug/uL.

**Type:** Secondary

**Prep By:** Alethea M. Shaules

**Status:** New

**Final Volume:** 50 mL

| Chemical/Solvent Used          | Bottle No    | Amt | Units | Expires  |
|--------------------------------|--------------|-----|-------|----------|
| Methanol, Purge and Trap EB373 | <u>14519</u> | 49  | mL    | 7/3/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0425     | ug/mL      | 1 mL         |



# Analytical RunID VOA5975C.I\_220104A Standards Traceability Report

**Spike ID:** VOCF3566A

**Spike Name:** 2nd Source Gases

**Prep Date:** 1/4/2022

**Exp Date:** 1/11/2022

**Department:** gcmsvoa

**Vendor:**

**Lot Number:**

**Balance ID:**

**Comments:** 1.0 ml/10 ml final volume. Final Concentration 0.2 ug/uL. Corrected final volume column to match comments and added final concentrations of analytes. MSC 01/14/2021

**Type:** Secondary

**Prep By:** Melissa Chavez

**Status:**

**Final Volume:** 10 mL

| Chemical/Solvent Used          | Bottle No    | Amt | Units | Expires   |
|--------------------------------|--------------|-----|-------|-----------|
| Methanol, Purge and Trap EB373 | <u>14519</u> | 9   | mL    | 1/11/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0417     | ug/mL      | 1 mL         |

# CERTIFICATE OF ANALYSIS

**Catalog No:** M-502A-R-10X  
**Description:** Volatile Organic Compounds - Liquids  
**Lot:** 220041126  
**Solvent:** Methanol  
**Hazards:** Refer to SDS for complete safety information

**Date Certified:** Apr 13, 2020  
**Expiration:** Apr 13, 2023  
**Sample Size:** 1 mL  
**Components:** 54  
**Storage Condition:** Refrig (0-5 °C)



Signal Word: Danger

Certified Reference Material



| Component                    | CAS #      | Purity % | Prepared                              | Certified Analyte                     |
|------------------------------|------------|----------|---------------------------------------|---------------------------------------|
|                              |            | (GC/MS)  | Concentration <sup>1</sup><br>(µg/mL) | Concentration <sup>1</sup><br>(µg/mL) |
| Benzene                      | 71-43-2    | 100.0    | 2002                                  | 2002                                  |
| Bromobenzene                 | 108-86-1   | 100.0    | 2003                                  | 2003                                  |
| Bromochloromethane           | 74-97-5    | 99.1     | 2001                                  | 1983                                  |
| Bromodichloromethane         | 75-27-4    | 99.0     | 2002                                  | 1982                                  |
| Bromoform                    | 75-25-2    | 99.2     | 2001                                  | 1985                                  |
| n-Butylbenzene               | 104-51-8   | 100.0    | 2002                                  | 2002                                  |
| sec-Butylbenzene             | 135-98-8   | 100.0    | 2001                                  | 2001                                  |
| tert-Butylbenzene            | 98-06-6    | 99.0     | 2003                                  | 1983                                  |
| Carbon tetrachloride         | 56-23-5    | 100.0    | 2003                                  | 2003                                  |
| Chlorobenzene                | 108-90-7   | 99.6     | 2001                                  | 1993                                  |
| Chloroform                   | 67-66-3    | 99.2     | 2004                                  | 1988                                  |
| 2-Chlorotoluene              | 95-49-8    | 99.0     | 2003                                  | 1983                                  |
| 4-Chlorotoluene              | 106-43-4   | 99.8     | 2002                                  | 1998                                  |
| Dibromochloromethane         | 124-48-1   | 97.8     | 2049*                                 | 2004                                  |
| 1,2-Dibromo-3-chloropropane  | 96-12-8    | 99.2     | 2001                                  | 1985                                  |
| 1,2-Dibromoethane            | 106-93-4   | 100.0    | 2006                                  | 2006                                  |
| Dibromomethane               | 74-95-3    | 99.0     | 2002                                  | 1982                                  |
| 1,2-Dichlorobenzene          | 95-50-1    | 98.2     | 2003                                  | 1967                                  |
| 1,3-Dichlorobenzene          | 541-73-1   | 100.0    | 2000                                  | 2000                                  |
| 1,4-Dichlorobenzene          | 106-46-7   | 100.0    | 2002                                  | 2002                                  |
| 1,1-Dichloroethane           | 75-34-3    | 98.6     | 2001                                  | 1973                                  |
| 1,2-Dichloroethane           | 107-06-2   | 99.8     | 2010                                  | 2006                                  |
| 1,1-Dichloroethene           | 75-35-4    | 99.0     | 2000                                  | 1980                                  |
| cis-1,2-Dichloroethene       | 156-59-2   | 99.0     | 2002                                  | 1982                                  |
| trans-1,2-Dichloroethene     | 156-60-5   | 99.5     | 2001                                  | 1991                                  |
| 1,2-Dichloropropane          | 78-87-5    | 99.5     | 2003                                  | 1993                                  |
| 1,3-Dichloropropane          | 142-28-9   | 96.7     | 2073*                                 | 2005                                  |
| 2,2-Dichloropropane          | 594-20-7   | 99.9     | 2012                                  | 2010                                  |
| 1,1-Dichloropropene          | 563-58-6   | 98.9     | 2001                                  | 1979                                  |
| cis-1,3-Dichloropropene **   | 10061-01-5 | 93.9     | 2041*                                 | 1916                                  |
| trans-1,3-Dichloropropene ** | 10061-02-6 | 93.9     | 1968*                                 | 1848                                  |
| Ethylbenzene                 | 100-41-4   | 99.7     | 2000                                  | 1994                                  |
| Hexachlorobutadiene          | 87-68-3    | 98.0     | 2003                                  | 1963                                  |
| Isopropylbenzene             | 98-82-8    | 100.0    | 2002                                  | 2002                                  |
| p-Isopropyltoluene           | 99-87-6    | 99.4     | 2000                                  | 1988                                  |
| Methylene chloride           | 75-09-2    | 99.9     | 2001                                  | 1999                                  |
| Naphthalene                  | 91-20-3    | 100.0    | 2002                                  | 2002                                  |
| n-Propylbenzene              | 103-65-1   | 100.0    | 2001                                  | 2001                                  |
| Styrene                      | 100-42-5   | 100.0    | 2003                                  | 2003                                  |
| 1,1,1,2-Tetrachloroethane    | 630-20-6   | 98.9     | 2005                                  | 1983                                  |
| 1,1,1,2,2-Tetrachloroethane  | 79-34-5    | 96.0     | 2087*                                 | 2004                                  |
| Tetrachloroethene            | 127-18-4   | 99.4     | 2017                                  | 2005                                  |
| Toluene                      | 108-88-3   | 100.0    | 2001                                  | 2001                                  |
| 1,2,3-Trichlorobenzene       | 87-61-6    | 100.0    | 2002                                  | 2002                                  |

# CERTIFICATE OF ANALYSIS

**Catalog No:** M-502A-R-10X  
**Description:** Volatile Organic Compounds - Liquids  
**Lot:** 220041126  
**Solvent:** Methanol

**Date Certified:** Apr 13, 2020  
**Expiration:** Apr 13, 2023  
**Sample Size:** 1 mL  
**Components:** 54

| Component - <i>continued</i> | CAS #    | Purity % | Prepared                              | Certified Analyte                     |
|------------------------------|----------|----------|---------------------------------------|---------------------------------------|
|                              |          | (GC/MS)  | Concentration <sup>2</sup><br>(µg/mL) | Concentration <sup>1</sup><br>(µg/mL) |
| 1,2,4-Trichlorobenzene       | 120-82-1 | 99.6     | 2001                                  | 1993                                  |
| 1,1,1-Trichloroethane        | 71-55-6  | 100.0    | 2002                                  | 2002                                  |
| 1,1,2-Trichloroethane        | 79-00-5  | 98.6     | 2000                                  | 1972                                  |
| Trichloroethene              | 79-01-6  | 100.0    | 2003                                  | 2003                                  |
| 1,2,3-Trichloropropane       | 96-18-4  | 97.5     | 2055*                                 | 2004                                  |
| 1,2,4-Trimethylbenzene       | 95-63-6  | 98.2     | 2001                                  | 1965                                  |
| 1,3,5-Trimethylbenzene       | 108-67-8 | 98.8     | 2001                                  | 1977                                  |
| o-Xylene                     | 95-47-6  | 99.0     | 2000                                  | 1980                                  |
| m-Xylene                     | 108-38-3 | 99.2     | 2002                                  | 1986                                  |
| p-Xylene                     | 106-42-3 | 95.4     | 2097*                                 | 2001                                  |

\* Weight compensated to 100% purity.

\*\* 47.8% cis isomer, 46.1% trans isomer

A product with a suffix (-1A, -2B, etc. or -01, -02, etc.) on its lot number has had its expiration date extended and is identical to the same lot number without the suffix.

<sup>2</sup> All weights are traceable through NIST, Test No. 684/289871-17

<sup>1</sup> Certified Analyte Concentration = Purity x Prepared Concentration.

The Uncertainty associated with the certified concentration reported on this certificate is  $\pm 2.4\%$ . This value is the combined expanded uncertainty and represents an estimated standard deviation equal to the positive square root of the total variation of the uncertainty of components. A normal distribution is assumed and a coverage factor of K=2 is chosen using approximately a 95% confidence level.

Labels and certificates follow U.S. Conventions in reporting numerical values: A comma (,) is used to separate units of one-thousand or greater. A period (.) is used as a decimal place marker.

The information on this certificate may not be reproduced without the express permission of the manufacturer. See reverse side for additional information

Certified By: 

Larry Decker, Organic QC Manager

**ID #:** 12797

Opened: \_\_\_\_\_

Volatile Organic Compounds - Liquids

**Expires:** 4/13/2023

Rec'd: 6/23/2020

Energy Laboratories Inc 1120 So. 27th Street  
Billings MT 59107

# Certificate of Analysis

**Product Name:** VOC Standard

**Product Number:** DWM-589N-1

**Lot Number:** 0006570990

**Lot Issue Date:** 17-Nov-2020

**Expiration Date:** 31-Dec-2023

**Description:**

This analytical reference material (RM) was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed below.

| Analyte                   | CAS#        | Analyte Lot | Concentration ± Uncertainty |
|---------------------------|-------------|-------------|-----------------------------|
| bromochloromethane        | 000074-97-5 | RM00009     | 2010 ± 10 µg/mL             |
| bromodichloromethane      | 000075-27-4 | RM12585     | 2009 ± 10 µg/mL             |
| bromoform                 | 000075-25-2 | RM13987     | 2010 ± 10 µg/mL             |
| carbon tetrachloride      | 000056-23-5 | RM07576     | 2010 ± 10 µg/mL             |
| chloroform                | 000067-66-3 | RM13988     | 2009 ± 10 µg/mL             |
| dibromochloromethane      | 000124-48-1 | RM14843     | 2009 ± 10 µg/mL             |
| dibromomethane            | 000074-95-3 | RM12878     | 2009 ± 10 µg/mL             |
| methylene chloride        | 000075-09-2 | RM11650     | 2009 ± 10 µg/mL             |
| 1,2-dibromoethane         | 000106-93-4 | RM00018     | 2010 ± 10 µg/mL             |
| 1,1-dichloroethane        | 000075-34-3 | RM16217     | 2006 ± 10 µg/mL             |
| 1,2-dichloroethane        | 000107-06-2 | RM04655     | 2005 ± 10 µg/mL             |
| 1,1-dichloroethene        | 000075-35-4 | RM14486     | 2010 ± 10 µg/mL             |
| cis-1,2-dichloroethene    | 000156-59-2 | RM15008     | 2007 ± 10 µg/mL             |
| trans-1,2-dichloroethene  | 000156-60-5 | RM07565     | 2008 ± 10 µg/mL             |
| 1,1,1,2-tetrachloroethane | 000630-20-6 | RM12632     | 2005 ± 10 µg/mL             |
| 1,1,2,2-tetrachloroethane | 000079-34-5 | RM02540     | 2009 ± 10 µg/mL             |
| tetrachloroethene         | 000127-18-4 | RM06491     | 2008 ± 10 µg/mL             |

# Certificate of Analysis

|                             |             |                    |                 |
|-----------------------------|-------------|--------------------|-----------------|
| <b>Product Number:</b>      | DWM-589N-1  | <b>Lot Number:</b> | 0006570990      |
| 1,1,1-trichloroethane       | 000071-55-6 | RM16539            | 2004 ± 10 µg/mL |
| 1,1,2-trichloroethane       | 000079-00-5 | RM01175            | 2009 ± 10 µg/mL |
| trichloroethene             | 000079-01-6 | RM14232            | 2009 ± 10 µg/mL |
| 1,2-dibromo-3-chloropropane | 000096-12-8 | RM13666            | 2009 ± 10 µg/mL |
| 1,2-dichloropropane         | 000078-87-5 | RM12821            | 2008 ± 10 µg/mL |
| 1,3-dichloropropane         | 000142-28-9 | RM02080            | 2008 ± 10 µg/mL |
| 2,2-dichloropropane         | 000594-20-7 | RM12927            | 2005 ± 10 µg/mL |
| 1,1-dichloropropene         | 000563-58-6 | RM16190            | 2010 ± 10 µg/mL |
| cis-1,3-dichloropropene     | 010061-01-5 | RM12891            | 2007 ± 10 µg/mL |
| trans-1,3-dichloropropene   | 010061-02-6 | RM12254            | 2006 ± 10 µg/mL |
| hexachlorobutadiene         | 000087-68-3 | RM09157            | 2005 ± 10 µg/mL |
| 1,2,3-trichloropropane      | 000096-18-4 | RM13082            | 2004 ± 10 µg/mL |
| benzene                     | 000071-43-2 | RM12931            | 2009 ± 10 µg/mL |
| n-butylbenzene              | 000104-51-8 | RM03651            | 2008 ± 10 µg/mL |
| sec-butylbenzene            | 000135-98-8 | RM10905            | 2005 ± 10 µg/mL |
| tert-butylbenzene           | 000098-06-6 | RM14040            | 2007 ± 10 µg/mL |
| ethylbenzene                | 000100-41-4 | RM12195            | 2006 ± 10 µg/mL |
| isopropylbenzene            | 000098-82-8 | RM00835            | 2009 ± 10 µg/mL |
| 4-isopropyltoluene          | 000099-87-6 | RM09747            | 2009 ± 10 µg/mL |
| naphthalene                 | 000091-20-3 | NT00970            | 2006 ± 10 µg/mL |
| n-propylbenzene             | 000103-65-1 | RM12785            | 2010 ± 10 µg/mL |
| styrene                     | 000100-42-5 | RM13393            | 2010 ± 10 µg/mL |



ISO 17034 Cert  
No. AR-1936

RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality Management System. Cert # 56 100 18560026

Page: 2 of 4

[www.agilent.com/quality/](http://www.agilent.com/quality/)  
CSD-QA-015.1



ISO 17025 Cert  
No. AT-1937



# Certificate of Analysis

**Product Number:** DWM-589N-1

**Lot Number:** 0006570990

|                        |             |         |                 |
|------------------------|-------------|---------|-----------------|
| toluene                | 000108-88-3 | RM06650 | 2008 ± 10 µg/mL |
| 1,2,4-trimethylbenzene | 000095-63-6 | RM06731 | 2002 ± 10 µg/mL |
| 1,3,5-trimethylbenzene | 000108-67-8 | RM12905 | 2009 ± 10 µg/mL |
| o-xylene               | 000095-47-6 | RM15639 | 2005 ± 10 µg/mL |
| m-xylene               | 000108-38-3 | RM15919 | 2006 ± 10 µg/mL |
| p-xylene               | 000106-42-3 | RM02647 | 2009 ± 10 µg/mL |
| bromobenzene           | 000108-86-1 | RM10227 | 2008 ± 10 µg/mL |
| chlorobenzene          | 000108-90-7 | RM01874 | 2008 ± 10 µg/mL |
| 2-chlorotoluene        | 000095-49-8 | RM13774 | 2007 ± 10 µg/mL |
| 4-chlorotoluene        | 000106-43-4 | RM11750 | 2009 ± 10 µg/mL |
| 1,2-dichlorobenzene    | 000095-50-1 | RM13636 | 2005 ± 10 µg/mL |
| 1,3-dichlorobenzene    | 000541-73-1 | NT00356 | 2009 ± 10 µg/mL |
| 1,4-dichlorobenzene    | 000106-46-7 | RM12826 | 2009 ± 10 µg/mL |
| 1,2,3-trichlorobenzene | 000087-61-6 | RM10193 | 2007 ± 10 µg/mL |
| 1,2,4-trichlorobenzene | 000120-82-1 | RM09454 | 2009 ± 10 µg/mL |

**Matrix:** methanol (methyl alcohol)

**Storage Conditions:** Store Frozen (-25° to -10°C).

**Traceability:**

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCCL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

**Homogeneity:**

This RM was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.



ISO 17034 Cert  
No. AR-1936

RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality Management System. Cert # 56 100 18560026

Page: 3 of 4

[www.agilent.com/quality/](http://www.agilent.com/quality/)  
CSD-QA-015.1



ISO 17025 Cert  
No. AT-1937

# Certificate of Analysis

Product Number: DWM-589N-1

Lot Number: 0006570990

## Intended Use:

This RM is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

## Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

## Hazards:

Refer to the Safety Data Sheet on [www.agilent.com](http://www.agilent.com) for information regarding this RM.

## Expiration of Certification:

The certification of this RM is valid until the expiration date specified above, provided the RM is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the RM is damaged, contaminated, or otherwise modified.

## Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:



Monica Bourgeois  
QMS Representative



ISO 17034 Cert  
No. AR-1936

RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality Management System. Cert # 56 100 18560026

Page: 4 of 4

[www.agilent.com/quality/](http://www.agilent.com/quality/)  
CSD-QA-015.1



ISO 17025 Cert  
No. AT-1937



*Jewar*

# CERTIFICATE OF ANALYSIS

**Catalog No:** M-8260A-B-SS-10X  
**Description:** Surrogate Standard Mix  
**Lot:** 219041458

**Solvent:** Methanol

**Hazards:** Refer to SDS for complete safety information

**Date Certified:** Apr 18, 2019  
**Expiration:** Apr 18, 2029  
**Sample Size:** 1 mL  
**Components:** 4  
**Storage Condition:** Ambient (>5 °C)



Signal Word: Danger

Certified Reference Material



| Component             | CAS #      | Purity %<br>(GC/MS) | Prepared<br>Concentration <sup>2</sup><br>(µg/mL) | Certified Analyte<br>Concentration <sup>1</sup><br>(µg/mL) |
|-----------------------|------------|---------------------|---------------------------------------------------|------------------------------------------------------------|
| p-Bromofluorobenzene  | 460-00-4   | 99.9                | 2004                                              | 2002                                                       |
| Dibromofluoromethane  | 1868-53-7  | 99.8                | 2005                                              | 2001                                                       |
| 1,2-Dichloroethane-d4 | 17060-07-0 | 100.0               | 2001                                              | 2001                                                       |
| Toluene-d8            | 2037-26-5  | 100.0               | 2000                                              | 2000                                                       |

**ID #: 13385**  
Opened: \_\_\_\_\_  
Surrogate Standard Mix  
**Expires: 4/18/2029**  
Rec'd: 1/4/2021  
Energy Laboratories Inc 1120 So. 27th Street  
Billings MT 59107

A product with a suffix (-1A, -2B, etc. or -01, -02, etc.) on its lot number has had its expiration date extended and is identical to the same lot number without the suffix.

<sup>2</sup> All weights are traceable through NIST, Test No. 684/289871-17

<sup>1</sup> Certified Analyte Concentration = Purity x Prepared Concentration.


The Uncertainty associated with the certified concentration reported on this certificate is ±2.4%. This value is the combined expanded uncertainty and represents an estimated standard deviation equal to the positive square root of the total variation of the uncertainty of components. A normal distribution is assumed and a coverage factor of K=2 is chosen using approximately a 95% confidence level.

Labels and certificates follow U.S. Conventions in reporting numerical values: A comma (,) is used to separate units of one-thousand or greater. A period (.) is used as a decimal place marker.

The information on this certificate may not be reproduced without the express permission of the manufacturer. See reverse side for additional information

Hazard Information: Please refer to the SDS for information regarding the hazards associated with using this material.

This product was prepared according to in-house procedures and is guaranteed to be homogeneous.

Certified By:   
Larry Decker, Organic QC Manager

# Certificate of Analysis

**Product Name:** Methyl tert-Butyl Ether Standard**Product Number:** STS-440-1**Lot Number:** 0006555762**Lot Issue Date:** 19-Aug-2020**Expiration Date:** 31-Aug-2022**Description:**

This analytical reference material (RM) was manufactured and verified in accordance with an ISO 9001 registered quality system, and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed below.

**Analyte****CAS#****Analyte Lot****Concentration ± Uncertainty**

tert-butylmethyl ether

001634-04-4

RM06568

2006 ± 10 µg/mL

**Matrix:** methanol (methyl alcohol)**Storage Conditions:** Store Frozen (-25° to -10°C).**Traceability:**

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCCL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

**Homogeneity:**

This RM was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

**Intended Use:**

This RM is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

**Instructions for Use:**

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

**Hazards:**

Refer to the Safety Data Sheet on [www.agilent.com](http://www.agilent.com) for information regarding this RM.

**Expiration of Certification:**

The certification of this RM is valid until the expiration date specified above, provided the RM is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the RM is damaged, contaminated, or otherwise modified.

**Maintenance of Certification:**

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

**Sample lot approver:**

Monica Bourgeois

QMS Representative

ISO 17034 Cert  
No. AR-1936RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality  
Management System. Cert # 56 100 18560026

Page: 1 of 1

[www.agilent.com/quality/](http://www.agilent.com/quality/)  
CSD-QA-015.1ISO 17025 Cert  
No. AT-1937

# CERTIFICATE OF ANALYSIS

Catalog No: S-078-10X

Description: MtBE

Lot: 220051182

Solvent: Methanol

Hazards: Refer to SDS for complete safety information

Date Certified: May 18, 2020

Expiration: May 18, 2030

Sample Size: 1 mL

Components: 1

Storage Condition: Ambient (>5 °C)



Signal Word: Danger

Certified Reference Material



| Component | CAS #     | Purity %<br>(GC/MS) | Prepared<br>Concentration <sup>2</sup><br>(µg/mL) | Certified Analyte<br>Concentration <sup>1</sup><br>(µg/mL) |
|-----------|-----------|---------------------|---------------------------------------------------|------------------------------------------------------------|
| MtBE      | 1634-04-4 | 100.0               | 2002                                              | 2002                                                       |

ID #: 13920

Opened: \_\_\_\_\_

MTBE

Expires: 5/18/2030

Rec'd: 6/7/2021

Energy Laboratories Inc 1120 So. 27th Street  
Billings MT 59107

A product with a suffix (-1A, -2B, etc. or -01, -02, etc.) on its lot number has had its expiration date extended and is identical to the same lot number without the suffix.

<sup>2</sup> All weights are traceable through NIST, Test No. 684/289871-17

<sup>1</sup> Certified Analyte Concentration = Purity x Prepared Concentration.

The Uncertainty associated with the certified concentration reported on this certificate is  $\pm 2.4\%$ . This value is the combined expanded uncertainty and represents an estimated standard deviation equal to the positive square root of the total variation of the uncertainty of components. A normal distribution is assumed and a coverage factor of K=2 is chosen using approximately a 95% confidence level.

Labels and certificates follow U.S. Conventions in reporting numerical values: A comma (,) is used to separate units of one-thousand or greater. A period (.) is used as a decimal place marker.

The information on this certificate may not be reproduced without the express permission of the manufacturer. See reverse side for additional information

Hazard Information: Please refer to the SDS for information regarding the hazards associated with using this material.

This product was prepared according to in-house procedures and is guaranteed to be homogeneous.

Certified By: \_\_\_\_\_

Larry Decker, Organic QC Manager

## CERTIFICATE OF ANALYSIS

CONCENTRATION 2000ug/ml in Methanol  
CATALOG NUMBER M-VOHC6M5-1ML  
LOT NUMBER 11882100  
DATE CERTIFIED 05/25/21  
EXPIRATION DATE 02/28/22  
STORAGE Store at room temperature (20 - 25 °C).  
HANDLING See Safety Data Sheet  
INTENDED USE For laboratory use only.  
ISO 17034:2016 CERTIFIED [ ]

### Volatile Organics High Concentration Mixture #6

ID #: 14142

Opened: \_\_\_\_\_

Volatile Organics High Concentration Mixture

Expires: 2/28/2022

Rec'd: 8/3/2021

Energx Laboratories Inc 1120 So. 27th Street  
Billings MT 59107

| ID      | Analyte                 | CAS     | Weight Analyte (mg) | Lot      | Purity | Certified Concentration (ug/mL) |
|---------|-------------------------|---------|---------------------|----------|--------|---------------------------------|
| N-11446 | Chloroethane            | 75-00-3 | 96.300              | 00001728 | 100.0  | 2006.3                          |
| N-11665 | Dichlorodifluoromethane | 75-71-8 | 96.610              | 00001729 | 100.0  | 2012.7                          |
| N-12417 | Methyl bromide          | 74-83-9 | 96.910              | 00024694 | 100.0  | 2019.0                          |
| N-12421 | Methyl chloride         | 74-87-3 | 96.150              | 00001731 | 100.0  | 2003.1                          |
| N-13655 | Trichlorofluoromethane  | 75-69-4 | 96.300              | 00027239 | 99.4   | 1994.2                          |
| N-13748 | Vinyl chloride          | 75-01-4 | 96.150              | 00019298 | 100.0  | 2003.1                          |

#### Analytical Test

#### Value

CONCENTRATION (GC/MSD)

VERIFIED

# CHEM SERVICE INC

660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599  
1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729  
[info@chemservice.com](mailto:info@chemservice.com) • [www.chemservice.com](http://www.chemservice.com)

## Instructions for Use:

Shake mixture prior to use. If particles are present, sonicate for homogeneity. If sample is diluted to lower concentrations, Class A volumetric glassware must be used.

Minimum Sample Size- 0.2 uL for Direct Injection.

Chem Service Inc. guarantees the expanded uncertainty of the above analytes to be +/- 2.0% of the certified concentrations based on gravimetric preparation. The test results published in this report were obtained using equipment capable of producing results that are traceable to NIST and through NIST to the International System of Units (SI). The reported expanded uncertainty of measurement is stated as the combined standard uncertainty of measurement multiplied by the coverage factor k (k=2) such that the coverage probability corresponds to approximately 95%. For certified reference materials, homogeneity and thermal stability testing are available upon request.

Certified By:

*Mary Beth O'Donnell*


Mary Beth O'Donnell  
CSM/TC



## CERTIFICATE OF ANALYSIS

### Analysis Method:

Catalog Number: M-VOHC6M5-1ML  
Description: Volatile Organics High Concentration Mixture #6  
Lot Number: 11882100  
Expiration Date: 02/28/22

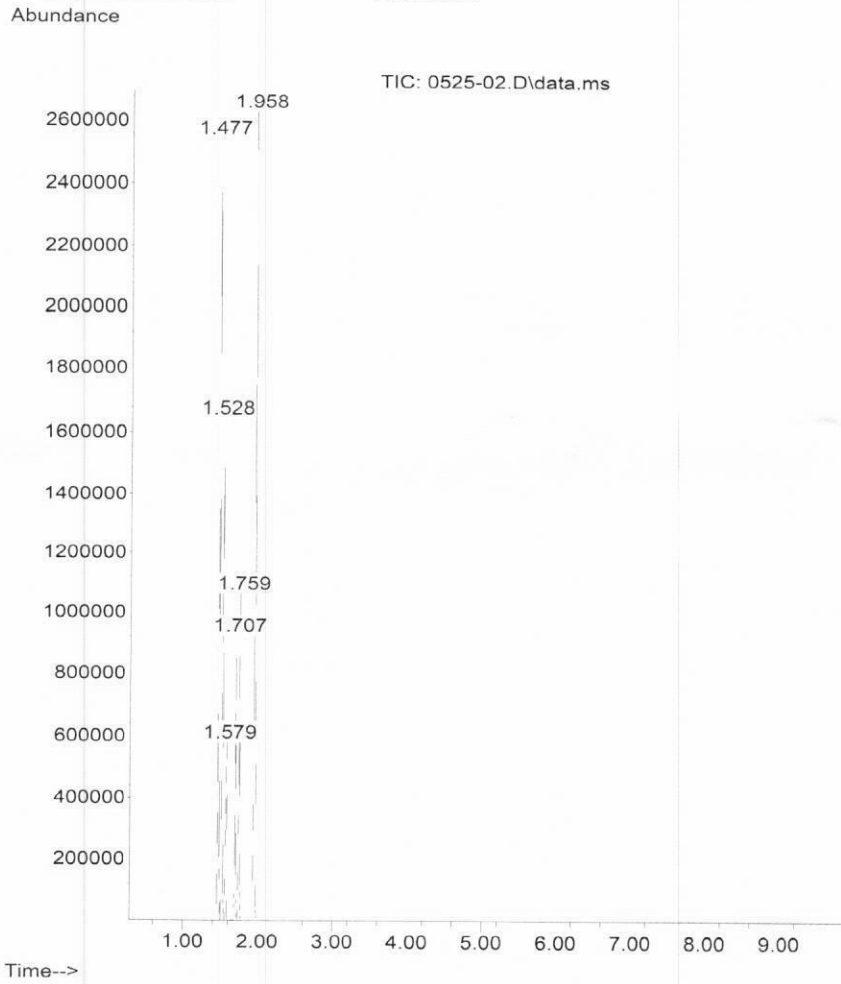



# Certificate of Analysis

ID #: 14251

Opened: \_\_\_\_\_

Internal Standard

Expires: 12/31/2022

Rec'd: 9/8/2021

Energy Laboratories Inc 1120 So. 27th Street  
Billings MT 59107

Product Name: Internal Standard

Product Number: STM-520-1

Lot Issue Date: 05-Jan-2021

Lot Number: 0006582580

Expiration Date: 31-Dec-2022

## Description:

This analytical reference material (RM) was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed below.

| Analyte                | CAS#        | Analyte Lot | Concentration ± Uncertainty |
|------------------------|-------------|-------------|-----------------------------|
| chlorobenzene-d5       | 003114-55-4 | RM12274     | 2501 ± 13 µg/mL             |
| 1,4-dichlorobenzene-d4 | 003855-82-1 | RM12517     | 2501 ± 13 µg/mL             |
| fluorobenzene          | 000462-06-6 | RM13378     | 2512 ± 13 µg/mL             |

Matrix: methanol (methyl alcohol)

Storage Conditions: Store Frozen (-25° to -10°C).

## Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCCL Z540.3, ISO 9001, ISO 17025 and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

## Homogeneity:

This RM was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

## Intended Use:

This RM is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

## Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

## Hazards:

Refer to the Safety Data Sheet on [www.agilent.com](http://www.agilent.com) for information regarding this RM.



ISO 17034  
REFERENCE MATERIAL  
PRODUCER  
ISO 17034 Cert  
No. AR-1936

RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality Management System. Cert # 56 100 18560026

Page: 1 of 2

[www.agilent.com/quality/](http://www.agilent.com/quality/)  
CSD-QA-015.1



ISO 17025 Cert  
No. AT-1937



# Certificate of Analysis

**Product Number:** STM-520-1

**Lot Number:** 0006582580

**Expiration of Certification:**

The certification of this RM is valid until the expiration date specified above, provided the RM is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the RM is damaged, contaminated, or otherwise modified.

**Maintenance of Certification:**

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

**Sample lot approver:**

Monica Bourgeois  
QMS Representative



ISO 17034 Cert  
No. AR-1936

RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality Management System. Cert # 56 100 18560026

Page: 2 of 2

[www.agilent.com/quality/](http://www.agilent.com/quality/)  
CSD-QA-015.1



ISO 17025 Cert  
No. AT-1937



# CERTIFICATE OF ANALYSIS

**Catalog No:** M-8260A-B-SS-10X  
**Description:** Surrogate Standard Mix  
**Lot:** 219041458

**Solvent:** Methanol

**Hazards:** Refer to SDS for complete safety information

**Date Certified:** Apr 18, 2019

**Expiration:** Apr 18, 2029

**Sample Size:** 1 mL

**Components:** 4

**Storage Condition:** Ambient (>5 °C)



Signal Word: Danger

## Certified Reference Material



| Component             | CAS #      | Purity %<br>(GC/MS) | Prepared<br>Concentration <sup>2</sup><br>(µg/mL) | Certified Analyte<br>Concentration <sup>1</sup><br>(µg/mL) |
|-----------------------|------------|---------------------|---------------------------------------------------|------------------------------------------------------------|
| p-Bromofluorobenzene  | 460-00-4   | 99.9                | 2004                                              | 2002                                                       |
| Dibromofluoromethane  | 1868-53-7  | 99.8                | 2005                                              | 2001                                                       |
| 1,2-Dichloroethane-d4 | 17060-07-0 | 100.0               | 2001                                              | 2001                                                       |
| Toluene-d8            | 2037-26-5  | 100.0               | 2000                                              | 2000                                                       |

**ID #:** 14269

Opened: \_\_\_\_\_

Surrogate Standard Mix

**Expires:** 4/18/2029

Rec'd: 9/14/2021

Energy Laboratories Inc 1120 So. 27th Street  
Billings MT 59107

A product with a suffix (-1A, -2B, etc. or -01, -02, etc.) on its lot number has had its expiration date extended and is identical to the same lot number without the suffix.

<sup>2</sup> All weights are traceable through NIST, Test No. 684/289871-17

<sup>1</sup> Certified Analyte Concentration = Purity x Prepared Concentration.

The Uncertainty associated with the certified concentration reported on this certificate is  $\pm 2.4\%$ . This value is the combined expanded uncertainty and represents an estimated standard deviation equal to the positive square root of the total variation of the uncertainty of components. A normal distribution is assumed and a coverage factor of K=2 is chosen using approximately a 95% confidence level.

Labels and certificates follow U.S. Conventions in reporting numerical values: A comma (,) is used to separate units of one-thousand or greater. A period (.) is used as a decimal place marker.



The information on this certificate may not be reproduced without the express permission of the manufacturer. See reverse side for additional information

Hazard Information: Please refer to the SDS for information regarding the hazards associated with using this material.

This product was prepared according to in-house procedures and is guaranteed to be homogeneous.

Certified By: \_\_\_\_\_

Larry Decker, Organic QC Manager



**CERTIFIED WEIGHT REPORT**

**Part Number:** 30058  
**Lot Number:** 080321  
**Description:** EPA Method 502/524 - Volatile Gases Mix #1

**Expiration Date:** 080324

**Recommended Storage:** Freezer (0 °C)

**Nominal Concentration (µg/mL):** 2000

**NIST Test ID#:** 6UTB

**Solvent:** Methanol  
**Lot#:** EA783-US

Weight(s) shown below were combined and diluted to (mL):  
500.0 0.058 Balance Uncertainty  
0.058 Flask Uncertainty


|                |                 |        |
|----------------|-----------------|--------|
|                |                 | 080321 |
| Formulated By: | Mario Luis      | DATE   |
|                |                 | 080321 |
| Reviewed By:   | Pedro L. Rentas | DATE   |

| Compound                   | RM# | Lot Number | Nominal Conc (µg/mL) | Purity (%) | Uncertainty Purity (%) | Target Weight (g) | Actual Weight (g) | Actual Conc(µg/mL) | Expanded Uncertainty (+/-) (µg/mL) | SDS Information (Solvent Safety Info. On Attached pg.) |                           |                   |
|----------------------------|-----|------------|----------------------|------------|------------------------|-------------------|-------------------|--------------------|------------------------------------|--------------------------------------------------------|---------------------------|-------------------|
|                            |     |            |                      |            |                        |                   |                   |                    |                                    | CAS#                                                   | OSHA PEL (TWA)            | LD50              |
| 1. Bromomethane            | 50  | 01611JX    | 2000                 | 99.5       | 0.2                    | 1.00508           | 1.0098            | 2009.4             | 8.1                                | 74-83-9                                                | 5 ppm (20mg/m3/8H) (skin) | ori-rat 214mg/kg  |
| 2. Chloroethane            | 72  | 062617     | 2000                 | 99         | 0.2                    | 1.01016           | 1.0146            | 2008.8             | 8.1                                | 75-00-3                                                | 1000 ppm (2600mg/m3/8H)   | N/A               |
| 3. Chloromethane           | 79  | 06908MS    | 2000                 | 99.5       | 0.2                    | 1.00508           | 1.0154            | 2020.5             | 8.1                                | 74-87-3                                                | 100 ppm                   | ori-rat 1800mg/kg |
| 4. Dichlorodifluoromethane | 134 | 92-0487    | 2000                 | 99         | 0.2                    | 1.01016           | 1.0224            | 2024.2             | 8.2                                | 75-71-8                                                | 1000 ppm (4950mg/m3/8H)   | N/A               |
| 5. Trichlorofluoromethane  | 294 | 01823MW    | 2000                 | 99         | 0.2                    | 1.01016           | 1.0110            | 2001.7             | 8.1                                | 75-69-4                                                | 1000 ppm (5600mg/m3/8H)   | ipr-mus 1743mg/kg |
| 6. Vinyl chloride          | 305 | 04854EA    | 2000                 | 99.5       | 0.2                    | 1.00508           | 1.0071            | 2004.0             | 8.1                                | 75-01-4                                                | N/A                       | N/A               |

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

**Comments**

GC15-M9 Analysis by Melissa Stonier  
Column ID SPB-Vocool 105 meter X 0.53mm X 3.0µm film thickness  
Flow rates: Total flow=150mL/min., Helium (carrier)=10mL/min., Helium(make-up)=40mL/min., Hydrogen(make-up)=100mL/min.  
Oven Profile: Temp. 1=35°C (Time 1=9 min.), Temp 2=200°C (Time 2=1 min.), Rate = 33°C/min., Total run time=15 min. Injector temp.=200°C, FID Temp.=200°C.  
ELCD Signal = Edaq Channel 1 PID Signal = Edaq Channel 2  
Standard injection = 0.5µL, Range=3 Purge Valve = 0 min.



| Peak No. | Analyte                 | ELCD RT (min.) |
|----------|-------------------------|----------------|
| 1        | Dichlorodifluoromethane | 4.67           |
| 2        | Chloromethane           | 5.28           |
| 3        | Vinyl chloride          | 5.56           |
| 4        | Bromomethane            | 6.75           |
| 5        | Chloroethane            | 6.99           |
| 6        | Trichlorofluoromethane  | 7.72           |

**ID #: 14285**

Opened: \_\_\_\_\_  
EPA Method 502-524 - Volatile Gases Mix #1  
**Expires: 8/3/2024**  
Rec'd: 9/17/2021  
Energy Laboratories Inc 1120 So. 27th Street  
Billings MT 59107

660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599  
1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729  
[info@chemservice.com](mailto:info@chemservice.com) • [www.chemservice.com](http://www.chemservice.com)

ID #: 14443

Opened: \_\_\_\_\_

TCL Ketone Mix

Expires: 6/30/2023

Rec'd: 10/26/2021

Energy Laboratories Inc 1120 So. 27th Street  
Billings MT 59107

## CERTIFICATE OF ANALYSIS

### TCL Ketones Mixture

CONCENTRATION 2000ug/ml in Methanol:Water (90:10)  
CATALOG NUMBER M-TCL1AN5-1ML  
LOT NUMBER 10251200  
DATE CERTIFIED 06/16/20  
EXPIRATION DATE 06/30/23  
STORAGE Freezer storage (-20 - -25 °C)  
HANDLING See Safety Data Sheet  
INTENDED USE For laboratory use only.  
ISO 17034:2016 CERTIFIED [ ]

| ID      | Analyte              | CAS      | Weight Analyte (mg) | Lot      | Purity | Certified Concentration (ug/mL) |
|---------|----------------------|----------|---------------------|----------|--------|---------------------------------|
| N-11014 | Acetone              | 67-64-1  | 203.300             | 00026182 | 98.7   | 2006.6                          |
| N-10297 | 2-Butanone           | 78-93-3  | 202.800             | 00027454 | 99.5   | 2017.9                          |
| N-10369 | 2-Hexanone           | 591-78-6 | 202.600             | 00025720 | 99.5   | 2015.9                          |
| N-10844 | 4-Methyl-2-pentanone | 108-10-1 | 204.700             | 6403300  | 99.5   | 2036.8                          |

| Analytical Test        | Value    |
|------------------------|----------|
| CONCENTRATION (GC/FID) | VERIFIED |

Chem Service, Inc. is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015.



COA Form  
Revision 3 (3/2015)

Print Date: 10/22/21

660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599  
1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729  
[info@chemservice.com](mailto:info@chemservice.com) • [www.chemservice.com](http://www.chemservice.com)

#### Instructions for Use:

Shake mixture prior to use. If particles are present, sonicate for homogeneity. If sample is diluted to lower concentrations, Class A volumetric glassware must be used.

Minimum Sample Size- 0.2 uL for Direct Injection.

Chem Service Inc. guarantees the expanded uncertainty of the above analytes to be +/- 2.0% of the certified concentrations based on gravimetric preparation. The test results published in this report were obtained using equipment capable of producing results that are traceable to NIST and through NIST to the International System of Units (SI). The reported expanded uncertainty of measurement is stated as the combined standard uncertainty of measurement multiplied by the coverage factor k (k=2) such that the coverage probability corresponds to approximately 95%. For certified reference materials, homogeneity and thermal stability testing are available upon request.

#### Certified By:

*Mary Beth O'Donnell*

Mary Beth O'Donnell  
CSM/TC

Chem Service, Inc. is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015.




660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599  
 1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729  
[info@chemservice.com](mailto:info@chemservice.com) • [www.chemservice.com](http://www.chemservice.com)

## CERTIFICATE OF ANALYSIS

Gas Chromatography / Flame Ionization Detector (GC/FID)

**Data file:** C:\CHEM321\DATA\2020 DATA\0620M-TCL1AN5.D  
**Sample name:** M-TCL1AN5  
**Acq. method:** N-14278.M  
**Instrument:** GC3  
**Injection date:** 6/16/2020 2:52:35 PM  
**Column name:** RTX-5MS (30m x 0.25mm x 0.5µm)  
**Location:** 202  
**Injection Vol:** 1.000  
**# Of Injections:** 1

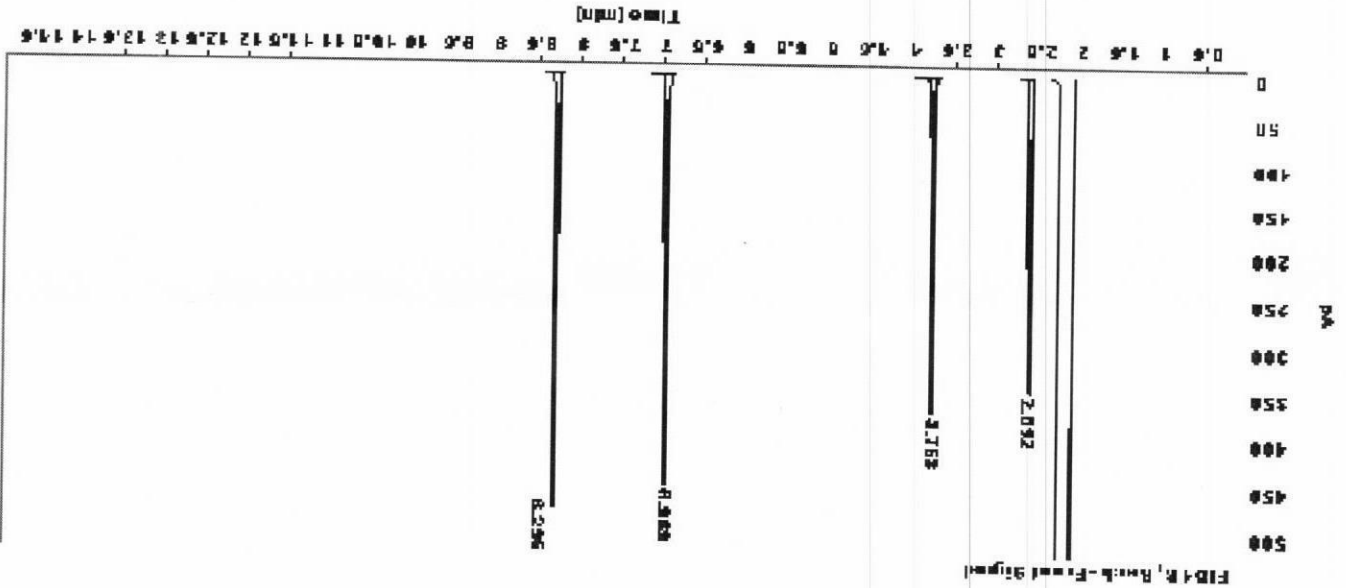

Signal: FID1 B, Back - Front Signal

| RT [min]  | Type | Width [min] | Area     | Height   | Area%   |
|-----------|------|-------------|----------|----------|---------|
| 2.592     | BB   | 0.0277      | 580.2505 | 343.4986 | 18.4655 |
| 3.763     | BB   | 0.0323      | 735.4804 | 387.8491 | 23.4054 |
| 6.969     | BB   | 0.0326      | 904.3389 | 447.8770 | 28.7791 |
| 8.295     | BB   | 0.0307      | 822.2798 | 474.3798 | 29.3500 |
| Sum       |      |             |          |          |         |
| 3142.3497 |      |             |          |          |         |

Chem Service, Inc. is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015.



# CERTIFICATE OF ANALYSIS

**Catalog No:** CLP-022K-10X  
**Description:** TCL Ketone Mix  
**Lot:** 221101480  
**Solvent:** Methanol  
**Hazards:** Refer to SDS for complete safety information

**Date Certified:** Oct 26, 2021  
**Expiration:** Nov 26, 2022  
**Sample Size:** 1 mL  
**Components:** 4  
**Storage Condition:** Freeze (<-10 °C)



**Certified Reference Material**



| Component            | CAS #    | Purity % | Prepared Concentration <sup>2</sup> | Certified Analyte Concentration <sup>1</sup> |
|----------------------|----------|----------|-------------------------------------|----------------------------------------------|
|                      |          | (GC/MS)  | (µg/mL)                             | (µg/mL)                                      |
| Acetone              | 67-64-1  | 100.0    | 2004                                | 2004                                         |
| 2-Butanone           | 78-93-3  | 100.0    | 2004                                | 2004                                         |
| 2-Hexanone           | 591-78-6 | 98.7     | 2004                                | 1978                                         |
| 4-Methyl-2-pentanone | 108-10-1 | 100.0    | 2004                                | 2004                                         |

**ID #: 14567**

Opened: \_\_\_\_\_

TCL Ketones Mixture

**Expires: 11/26/2022**

Rec'd: 11/30/2021

Energy Laboratories Inc 1120 So. 27th Street  
Billings MT 59107

This Certified Reference Material was verified in accordance with ISO/IEC 17025

A product with a suffix (-1A, -2B, etc. or -01, -02, etc.) on its lot number has had its expiration date extended and is identical to the same lot number without the suffix.

<sup>2</sup> All weights are traceable through NIST, Test No. 684/289871-17

<sup>1</sup> Certified Analyte Concentration = Purity x Prepared Concentration.

The Uncertainty associated with the certified concentration reported on this certificate is  $\pm 2.4\%$ . This value is the combined expanded uncertainty and represents an estimated standard deviation equal to the positive square root of the total variation of the uncertainty of components. A normal distribution is assumed and a coverage factor of K=2 is chosen using approximately a 95% confidence level.

Labels and certificates follow U.S. Conventions in reporting numerical values: A comma (,) is used to separate units of one-thousand or greater. A period (.) is used as a decimal place marker.

The information on this certificate may not be reproduced without the express permission of the manufacturer. See reverse side for additional information

Hazard Information: Please refer to the SDS for information regarding the hazards associated with using this material.

This product was prepared according to in-house procedures and is guaranteed to be homogeneous.

Certified By: \_\_\_\_\_

Larry Decker, Organic QC Manager

# CERTIFICATE OF ANALYSIS

**Catalog No:** CLP-022K-10X  
**Description:** TCL Ketone Mix  
**Lot:** 221101480  
**Solvent:** Methanol

**Date Certified:** Oct 26, 2021  
**Expiration:** Nov 26, 2022  
**Sample Size:** 1 mL  
**Components:** 4

## T-Test

AccuStandard, Inc.  
Statistical Report for CLP (SOW 1391)  
26-Oct-2021

QR-QC-003 rev. 1/16

| CLP-022K-10X<br>221101480 |                                 |        |        |        |        |      |         |       |        |        |        | CLP-022K-10X<br>221041075 |      |         |       |            |       |                                 |      |           |                           |     |  | NOTES: |  |  |  |
|---------------------------|---------------------------------|--------|--------|--------|--------|------|---------|-------|--------|--------|--------|---------------------------|------|---------|-------|------------|-------|---------------------------------|------|-----------|---------------------------|-----|--|--------|--|--|--|
| RT                        | Component                       | Run #1 | Run #2 | Run #3 | Run #4 | Mean | Std Dev | % RSD | Run #1 | Run #2 | Run #3 | Run #4                    | Mean | Std Dev | % RSD | t.025 test | CI    | Component                       | CI   | # of Runs | 10 % error check of Conc. |     |  |        |  |  |  |
| 3.74                      | Acetone (67-64-1)               | 1925   | 1881   | 1854   | 1803   | 1866 | 51.05   | 2.74% | 1751   | 1712   | 1730   | 1764                      | 1764 | 22.43   | 1.29% | 4.36       | 119.2 | Acetone (67-64-1)               | 56   | 4         | 2000                      | 7 % |  |        |  |  |  |
| 5.77                      | 2-Butanone (78-93-3)            | 2275   | 2223   | 2237   | 2149   | 2221 | 52.79   | 2.38% | 2157   | 2103   | 2145   | 2177                      | 2146 | 31.26   | 1.45% | 2.46       | 58.5  | 2-Butanone (78-93-3)            | 35.9 | 4         | 2000                      | 9 % |  |        |  |  |  |
| 8.34                      | 4-Methyl-2-pentanone (108-10-1) | 3373   | 3302   | 3408   | 3225   | 3327 | 81.05   | 2.44% | 3349   | 3240   | 3296   | 3415                      | 3325 | 74.70   | 2.25% | 0.04       | 0.9   | 4-Methyl-2-pentanone (108-10-1) | 0.8  | 4         | 2000                      | 0 % |  |        |  |  |  |
| 9.13                      | 2-Hexanone (99-178-6)           | 3260   | 3199   | 3332   | 3118   | 3227 | 90.88   | 2.62% | 3186   | 3072   | 3120   | 3239                      | 3154 | 73.32   | 2.32% | 1.25       | 35.2  | 2-Hexanone (99-178-6)           | 29.1 | 4         | 2000                      | 2 % |  |        |  |  |  |


# CERTIFICATE OF ANALYSIS

**Catalog No:** CLP-022K-10X  
**Description:** TCL Ketone Mix  
**Lot:** 221101480  
**Solvent:** Methanol


**Date Certified:** Oct 26, 2021  
**Expiration:** Nov 26, 2022  
**Sample Size:** 1 mL  
**Components:** 4

## Chromatogram

File : Q:\GCMS-06 Minimal\DATA\102521\13- 221101480 KM.D  
Operator : Organic QC Lab  
Acquired : 25 Oct 2021 21:00 using AcqMethod VOC-Split100.M  
Instrument : GCMS 6  
Sample Name : CLP-022K-10X (221101480)  
Misc Info : TCL Ketone Mix @ 2000 ug/mL in MeOH  
Vial Number : 34



Column: DB-624 UI, 30m x 0.25mm ID x 1.4µm  
Oven Program: 35°C (hold 5min), 11°C/min to 60°C, 22°C/min to 230°C (hold 4min)  
GC Parameters: Split 100:1, 1µl inj.; GC/MS; injector temp 240°C







# Analytical RunID VOA5975C.I\_220107A Standards Traceability Report

**Standard ID:** VOCF0313

**Standard Name:** Liquids

**Prep Date:** 6/23/2020

**Exp Date:** 4/13/2023

**Department:** gcmsvoa

**Vendor:** AccuStd

**Lot Number:** 220041126

**Balance ID:**

**Comments:** Date Prepared is same as Date Received. 2,000 ug/mL. Catalog # M502A-R-10X. Corrected lot number to match Cl. MSC 01/14/2022

**Type:** Primary

**Prep By:** Alethea M. Shaules

**Status:** New

**Final Volume:** 10 mL

| Chemical/Solvent Used                | Bottle No    | Amt | Units | Expires   |
|--------------------------------------|--------------|-----|-------|-----------|
| Volatile Organic Compounds - Liquids | <u>12797</u> | 1   | mL    | 4/13/2023 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0313     | ug/mL      |              |



# Analytical RunID VOA5975C.I\_220107A Standards Traceability Report

**Spike ID:** VOCF0352

**Spike Name:** 2nd Source Liquids

**Prep Date:** 11/23/2020

**Exp Date:** 12/31/2023

**Department:** gcmsvoa

**Vendor:** Agilent

**Lot Number:** 0006570990

**Balance ID:**

**Comments:** Date Prepared is same as Date Received. 2000 ug/mL in MeOH. Catalog # DWM-589N-1.

**Type:** Primary

**Prep By:** Steve Dilts

**Status:** New

**Final Volume:** 10 mL

| Chemical/Solvent Used | Bottle No    | Amt | Units | Expires    |
|-----------------------|--------------|-----|-------|------------|
| VOC Standard          | <u>13292</u> | 1   | mL    | 12/31/2023 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0352     | ug/mL      |              |



# Analytical RunID VOA5975C.I\_220107A Standards Traceability Report

**Standard ID:** VOCF0373

**Standard Name:** MtBE (Methy tert-Butyl Ether)

**Prep Date:** 2/26/2021

**Exp Date:** 8/31/2022

**Department:** gcmsvoa

**Vendor:** Agilent

**Lot Number:** 0006555762

**Balance ID:**

**Comments:** Date Prepared is same as Date Received. 2000 ug/mL in MeOH. Catalog # STS-440

**Type:** Primary

**Prep By:** Steve Dilts

**Status:** New

**Final Volume:** 5 mL

| Chemical/Solvent Used            | Bottle No | Amt | Units | Expires   |
|----------------------------------|-----------|-----|-------|-----------|
| Methyl tert-Butyl Ether Standard | 13578     | 1   | mL    | 8/31/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0373     | ug/mL      |              |



# Analytical RunID VOA5975C.I\_220107A Standards Traceability Report

**Spike ID:** VOCF0401

**Spike Name:** 2nd Source MtBE

**Prep Date:** 6/7/2021

**Exp Date:** 12/11/2029

**Department:** gcmsvoa

**Vendor:** AccuStandard

**Lot Number:** 220051182

**Balance ID:**

**Comments:** Date Prepared is same as Date Receive. 2,000 ug/mL in MeOH. Catalog # S-078-10X.

**Type:** Primary

**Prep By:** Alethea M. Shaules

**Status:** New

**Final Volume:** 5 mL

| Chemical/Solvent Used | Bottle No | Amt | Units | Expires    |
|-----------------------|-----------|-----|-------|------------|
| MTBE                  | 13920     | 1   | mL    | 12/11/2029 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0401     | ug/mL      |              |



# Analytical RunID VOA5975C.I\_220107A Standards Traceability Report

**Spike ID:** VOCF0417

**Spike Name:** Chem Service Gases

**Type:** Primary

**Prep Date:** 8/3/2021

**Prep By:** Steve Dilts

**Exp Date:** 2/28/2022

**Status:**

**Department:** gcmsvoa

**Vendor:** Chemservice

**Final Volume:** 5 mL

**Lot Number:** 11882100

**Balance ID:**

**Comments:** Date Prepared is same as Date Received. 2000 ug/mL in MeOH. Catalog # M-VOHC6M5-1ML

| Chemical/Solvent Used                           | Bottle No    | Amt | Units | Expires   |
|-------------------------------------------------|--------------|-----|-------|-----------|
| Volatile Organics High Concentration Mixture #6 | <u>14142</u> | 5   | mL    | 2/28/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0417     | ug/mL      |              |



# Analytical RunID VOA5975C.I\_220107A Standards Traceability Report

**Standard ID:** VOCF0425

**Standard Name:** Internals

**Prep Date:** 9/8/2021

**Exp Date:** 12/31/2022

**Department:** gcmsvoa

**Vendor:** Agilent

**Lot Number:** 0006582580

**Balance ID:**

**Comments:** Date Prepared is same as Date Received. 2,500 ug/mL in MeOH. Catalog # STM-520-1.

**Type:** Primary

**Prep By:** Jerran D. Brenden

**Status:** New

**Final Volume:** 10 mL

| Chemical/Solvent Used | Bottle No    | Amt | Units | Expires    |
|-----------------------|--------------|-----|-------|------------|
| Internal Standard     | <u>14251</u> | 1   | mL    | 12/31/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0425     | ug/mL      |              |



# Analytical RunID VOA5975C.I\_220107A Standards Traceability Report

**Spike ID:** VOCF0426

**Spike Name:** Surrogates 2.0 mg/mL

**Prep Date:** 9/14/2021

**Exp Date:** 4/18/2029

**Department:** gcmsvoa

**Vendor:** AccuStandard

**Lot Number:** 219041458

**Balance ID:**

**Comments:** Date Received 01/04/2021. 2.0 mg/mL. Catalog # M-8260A-B-SS-10X

**Type:** Primary

**Prep By:** Jerran D. Brenden

**Status:** New

**Final Volume:** 10 mL

| Chemical/Solvent Used  | Bottle No    | Amt | Units | Expires   |
|------------------------|--------------|-----|-------|-----------|
| Surrogate Standard Mix | <u>14269</u> | 1   | mL    | 4/18/2029 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0426     | ug/mL      |              |



# Analytical RunID VOA5975C.I\_220107A Standards Traceability Report

**Standard ID:** VOCF0427

**Standard Name:** Gases

**Prep Date:** 9/17/2021

**Exp Date:** 8/3/2024

**Department:** gcmsvoa

**Vendor:** Absolute

**Lot Number:** 080321

**Balance ID:**

**Comments:** Date Prepared is same as Date Received. 2,000 ug/mL in MeOH. Catalog # 30058.

**Type:** Primary

**Prep By:** Alethea M. Shaules

**Status:** New

**Final Volume:** 10 mL

| Chemical/Solvent Used                      | Bottle No    | Amt | Units | Expires  |
|--------------------------------------------|--------------|-----|-------|----------|
| EPA Method 502-524 - Volatile Gases Mix #1 | <u>14285</u> | 1   | mL    | 8/3/2024 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0427     | ug/mL      |              |





# Analytical RunID VOA5975C.I\_220107A Standards Traceability Report

**Standard ID:** VOCF0434

**Standard Name:** Ketones

**Prep Date:** 10/26/2021

**Exp Date:** 6/30/2023

**Department:** gcmsvoa

**Vendor:** Chem Service

**Lot Number:** 10251200

**Balance ID:**

**Comments:** Date Prepared is same as Date Received. 2,000 ug/mL in 90:10 MeOH:H2O. Catalog # M-TCL-1AN5-5ML.

**Type:** Primary

**Prep By:** Steve Dilts

**Status:** New

**Final Volume:** 5 mL

| Chemical/Solvent Used | Bottle No    | Amt | Units | Expires   |
|-----------------------|--------------|-----|-------|-----------|
| TCL Ketone Mix        | <u>14443</u> | 1   | mL    | 6/30/2023 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0434     | ug/mL      |              |



# Analytical RunID VOA5975C.I\_220107A Standards Traceability Report

**Standard ID:** VOCF0439

**Standard Name:** 2nd Source Ketones

**Prep Date:** 11/30/2021

**Exp Date:** 11/26/2022

**Department:** gcmsvoa

**Vendor:** AccuStandard

**Lot Number:** 221101480

**Balance ID:**

**Comments:** Date Prepared is same as Date Received. 2,000 ug/mL in Methanol. Catalog # CLP-022K-10X.

**Type:** Primary

**Prep By:** Melissa Chavez

**Status:** New

**Final Volume:** 1 mL

| Chemical/Solvent Used | Bottle No    | Amt | Units | Expires    |
|-----------------------|--------------|-----|-------|------------|
| TCL Ketones Mixture   | <u>14567</u> | 2   | mL    | 11/26/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0439     | ug/mL      |              |



# Analytical RunID VOA5975C.I\_220107A Standards Traceability Report

**Spike ID:** VOCF3517

**Spike Name:** Internal Standard / Surrogates (INT/SURR)

**Type:** Secondary

**Prep Date:** 11/10/2021

**Prep By:** Alethea M. Shaules

**Exp Date:** 12/31/2022

**Status:** New

**Department:** gcmsvoa

**Vendor:**

**Final Volume:** 100 mL

**Lot Number:**

**Balance ID:**

**Comments:** Final Concentration 0.05 ug/uL in MeOH.

| Chemical/Solvent Used               | Bottle No    | Amt  | Units | Expires    |
|-------------------------------------|--------------|------|-------|------------|
| Methanol, Purge and Trap - EB199-US | <u>14334</u> | 95.5 | mL    | 12/31/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0425     | ug/mL      | 2 mL         |
| VOCF0426     | ug/mL      | 2.5 mL       |



# Analytical RunID VOA5975C.I\_220107A Standards Traceability Report

**Spike ID:** VOCF3529B

**Spike Name:** 2nd Source MtBE

**Prep Date:** 11/29/2021

**Exp Date:** 1/29/2022

**Department:** gcmsvoa

**Vendor:**

**Lot Number:**

**Balance ID:**

**Comments:** Final Concentration 0.2 ug/uL

**Type:** Secondary

**Prep By:** Alethea M. Shaules

**Status:**

**Final Volume:** 10 mL

| Chemical/Solvent Used               | Bottle No    | Amt | Units | Expires   |
|-------------------------------------|--------------|-----|-------|-----------|
| Methanol, Purge and Trap - EB199-US | <u>14334</u> | 9   | mL    | 1/29/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0401     | ug/mL      | 1 mL         |



# Analytical RunID VOA5975C.I\_220107A Standards Traceability Report

**Standard ID:** VOFC3546A

**Standard Name:** Liquids

**Prep Date:** 12/13/2021

**Exp Date:** 1/13/2022

**Department:** GCMSVOA

**Vendor:**

**Lot Number:**

**Balance ID:**

**Comments:** 1.0 ml/10 ml final volume. Final Concentration 0.2 ug/uL. Corrected comment and analyte list 11/9/2021 sbd

**Type:** Secondary

**Prep By:** Alethea M. Shaules

**Status:**

**Final Volume:** 10 mL

| Chemical/Solvent Used          | Bottle No    | Amt | Units | Expires   |
|--------------------------------|--------------|-----|-------|-----------|
| Methanol, Purge and Trap EA899 | <u>13926</u> | 9   | mL    | 1/13/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0313     | ug/mL      | 1 mL         |



# Analytical RunID VOA5975C.I\_220107A Standards Traceability Report

**Spike ID:** VOCF3549

**Spike Name:** 2nd Source Ketones

**Prep Date:** 12/15/2021

**Exp Date:** 1/15/2022

**Department:** gcmsvoa

**Vendor:** AccuStandard

**Lot Number:** 221101480

**Balance ID:**

**Comments:** Vial opened for use. 2.0 µg/µL

**Type:** Primary

**Prep By:** Melissa Chavez

**Status:**

**Final Volume:** 1 mL

| Chemical/Solvent Used | Bottle No    | Amt | Units | Expires   |
|-----------------------|--------------|-----|-------|-----------|
| TCL Ketones Mixture   | <u>14567</u> | 1   | mL    | 1/15/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0439     | ug/mL      | 1 mL         |



# Analytical RunID VOA5975C.I\_220107A Standards Traceability Report

**Standard ID:** VOCF3550

**Standard Name:** Ketones

**Prep Date:** 12/16/2021

**Exp Date:** 1/16/2022

**Department:** gcmsvoa

**Vendor:** Chem Service

**Lot Number:** 10251200

**Balance ID:**

**Comments:** Vial Opened For Use . 2.0 ug/uL in 90:10 MeOH:H2O.

**Type:** Primary

**Prep By:** Melissa Chavez

**Status:**

**Final Volume:** 1 mL

| Chemical/Solvent Used | Bottle No    | Amt | Units | Expires   |
|-----------------------|--------------|-----|-------|-----------|
| TCL Ketone Mix        | <u>14443</u> | 1   | mL    | 1/16/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0434     | ug/mL      | 1 mL         |



# Analytical RunID VOA5975C.I\_220107A Standards Traceability Report

**Spike ID:** VOCF3558B

**Spike Name:** 2nd Source Liquids

**Type:** Secondary

**Prep Date:** 12/27/2021

**Prep By:** Steve Dilts

**Exp Date:** 2/27/2022

**Status:** Open

**Department:** gcmsvoa

**Vendor:**

**Final Volume:** 10 mL

**Lot Number:**

**Balance ID:**

**Comments:** Final Concentration 0.2ug/uL.

| Chemical/Solvent Used               | Bottle No    | Amt | Units | Expires   |
|-------------------------------------|--------------|-----|-------|-----------|
| Methanol, Purge and Trap - EB199-US | <u>14334</u> | 9   | mL    | 2/27/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0352     | ug/mL      | 1 mL         |





# Analytical RunID VOA5975C.I\_220107A Standards Traceability Report

**Standard ID:** VOCF3559A

**Standard Name:** MtBE

**Prep Date:** 12/27/2021

**Exp Date:** 1/27/2022

**Department:** gcmsvoa

**Vendor:**

**Lot Number:**

**Balance ID:**

**Comments:** Final Concentration 0.2 ug/uL.

**Type:** Secondary

**Prep By:** Melissa Chavez

**Status:**

**Final Volume:** 10 mL

| Chemical/Solvent Used               | Bottle No    | Amt | Units | Expires   |
|-------------------------------------|--------------|-----|-------|-----------|
| Methanol, Purge and Trap - EB199-US | <u>14334</u> | 9   | mL    | 1/27/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0373     | ug/mL      | 1 mL         |



# Analytical RunID VOA5975C.I\_220107A Standards Traceability Report

**Standard ID:** VOCF3562A

**Standard Name:** Gases

**Prep Date:** 1/3/2022

**Exp Date:** 1/10/2022

**Department:** GCMSVOA

**Vendor:**

**Lot Number:**

**Balance ID:**

**Comments:** 1.0 ml/10 ml final volume. Final Concentration 0.2 ug/uL

**Type:** Secondary

**Prep By:** Alethea M. Shaules

**Status:**

**Final Volume:** 10 mL

| Chemical/Solvent Used          | Bottle No    | Amt | Units | Expires   |
|--------------------------------|--------------|-----|-------|-----------|
| Methanol, Purge and Trap EB373 | <u>14519</u> | 9   | mL    | 1/10/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0427     | ug/mL      | 1 mL         |



# Analytical RunID VOA5975C.I\_220107A Standards Traceability Report

**Spike ID:** VOCF3566A

**Spike Name:** 2nd Source Gases

**Prep Date:** 1/4/2022

**Exp Date:** 1/11/2022

**Department:** gcmsvoa

**Vendor:**

**Lot Number:**

**Balance ID:**

**Comments:** 1.0 ml/10 ml final volume. Final Concentration 0.2 ug/uL. Corrected final volume column to match comments and added final concentrations of analytes. MSC 01/14/2021

**Type:** Secondary

**Prep By:** Melissa Chavez

**Status:**

**Final Volume:** 10 mL

| Chemical/Solvent Used          | Bottle No    | Amt | Units | Expires   |
|--------------------------------|--------------|-----|-------|-----------|
| Methanol, Purge and Trap EB373 | <u>14519</u> | 9   | mL    | 1/11/2022 |

| Stock Source | Base Units | Amount Added |
|--------------|------------|--------------|
| VOCF0417     | ug/mL      | 1 mL         |

# CERTIFICATE OF ANALYSIS

**Catalog No:** M-502A-R-10X  
**Description:** Volatile Organic Compounds - Liquids  
**Lot:** 220041126  
**Solvent:** Methanol  
**Hazards:** Refer to SDS for complete safety information

**Date Certified:** Apr 13, 2020  
**Expiration:** Apr 13, 2023  
**Sample Size:** 1 mL  
**Components:** 54  
**Storage Condition:** Refrig (0-5 °C)



Signal Word: Danger

Certified Reference Material



| Component                    | CAS #      | Purity %<br>(GC/MS) | Prepared Concentration*<br>(µg/mL) | Certified Analyte Concentration*<br>(µg/mL) |
|------------------------------|------------|---------------------|------------------------------------|---------------------------------------------|
| Benzene                      | 71-43-2    | 100.0               | 2002                               | 2002                                        |
| Bromobenzene                 | 108-86-1   | 100.0               | 2003                               | 2003                                        |
| Bromochloromethane           | 74-97-5    | 99.1                | 2001                               | 1983                                        |
| Bromodichloromethane         | 75-27-4    | 99.0                | 2002                               | 1982                                        |
| Bromoform                    | 75-25-2    | 99.2                | 2001                               | 1985                                        |
| n-Butylbenzene               | 104-51-8   | 100.0               | 2002                               | 2002                                        |
| sec-Butylbenzene             | 135-98-8   | 100.0               | 2001                               | 2001                                        |
| tert-Butylbenzene            | 98-06-6    | 99.0                | 2003                               | 1983                                        |
| Carbon tetrachloride         | 56-23-5    | 100.0               | 2003                               | 2003                                        |
| Chlorobenzene                | 108-90-7   | 99.6                | 2001                               | 1993                                        |
| Chloroform                   | 67-66-3    | 99.2                | 2004                               | 1988                                        |
| 2-Chlorotoluene              | 95-49-8    | 99.0                | 2003                               | 1983                                        |
| 4-Chlorotoluene              | 106-43-4   | 99.8                | 2002                               | 1998                                        |
| Dibromochloromethane         | 124-48-1   | 97.8                | 2049*                              | 2004                                        |
| 1,2-Dibromo-3-chloropropane  | 96-12-8    | 99.2                | 2001                               | 1985                                        |
| 1,2-Dibromoethane            | 106-93-4   | 100.0               | 2006                               | 2006                                        |
| Dibromomethane               | 74-95-3    | 99.0                | 2002                               | 1982                                        |
| 1,2-Dichlorobenzene          | 95-50-1    | 98.2                | 2003                               | 1967                                        |
| 1,3-Dichlorobenzene          | 541-73-1   | 100.0               | 2000                               | 2000                                        |
| 1,4-Dichlorobenzene          | 106-46-7   | 100.0               | 2002                               | 2002                                        |
| 1,1-Dichloroethane           | 75-34-3    | 98.6                | 2001                               | 1973                                        |
| 1,2-Dichloroethane           | 107-06-2   | 99.8                | 2010                               | 2006                                        |
| 1,1-Dichloroethene           | 75-35-4    | 99.0                | 2000                               | 1980                                        |
| cis-1,2-Dichloroethene       | 156-59-2   | 99.0                | 2002                               | 1982                                        |
| trans-1,2-Dichloroethene     | 156-60-5   | 99.5                | 2001                               | 1991                                        |
| 1,2-Dichloropropane          | 78-87-5    | 99.5                | 2003                               | 1993                                        |
| 1,3-Dichloropropane          | 142-28-9   | 96.7                | 2073*                              | 2005                                        |
| 2,2-Dichloropropane          | 594-20-7   | 99.9                | 2012                               | 2010                                        |
| 1,1-Dichloropropene          | 563-58-6   | 98.9                | 2001                               | 1979                                        |
| cis-1,3-Dichloropropene **   | 10061-01-5 | 93.9                | 2041*                              | 1916                                        |
| trans-1,3-Dichloropropene ** | 10061-02-6 | 93.9                | 1968*                              | 1848                                        |
| Ethylbenzene                 | 100-41-4   | 99.7                | 2000                               | 1994                                        |
| Hexachlorobutadiene          | 87-68-3    | 98.0                | 2003                               | 1963                                        |
| Isopropylbenzene             | 98-82-8    | 100.0               | 2002                               | 2002                                        |
| p-Isopropyltoluene           | 99-87-6    | 99.4                | 2000                               | 1988                                        |
| Methylene chloride           | 75-09-2    | 99.9                | 2001                               | 1999                                        |
| Naphthalene                  | 91-20-3    | 100.0               | 2002                               | 2002                                        |
| n-Propylbenzene              | 103-65-1   | 100.0               | 2001                               | 2001                                        |
| Styrene                      | 100-42-5   | 100.0               | 2003                               | 2003                                        |
| 1,1,1,2-Tetrachloroethane    | 630-20-6   | 98.9                | 2005                               | 1983                                        |
| 1,1,2,2-Tetrachloroethane    | 79-34-5    | 96.0                | 2087*                              | 2004                                        |
| Tetrachloroethene            | 127-18-4   | 99.4                | 2017                               | 2005                                        |
| Toluene                      | 108-88-3   | 100.0               | 2001                               | 2001                                        |
| 1,2,3-Trichlorobenzene       | 87-61-6    | 100.0               | 2002                               | 2002                                        |

# CERTIFICATE OF ANALYSIS

**Catalog No:** M-502A-R-10X  
**Description:** Volatile Organic Compounds - Liquids  
**Lot:** 220041126  
**Solvent:** Methanol

**Date Certified:** Apr 13, 2020  
**Expiration:** Apr 13, 2023  
**Sample Size:** 1 mL  
**Components:** 54

| Component - <i>continued</i> | CAS #    | Purity % | Prepared Concentration <sup>2</sup> | Certified Analyte Concentration <sup>1</sup> |
|------------------------------|----------|----------|-------------------------------------|----------------------------------------------|
|                              |          | (GC/MS)  | (µg/mL)                             | (µg/mL)                                      |
| 1,2,4-Trichlorobenzene       | 120-82-1 | 99.6     | 2001                                | 1993                                         |
| 1,1,1-Trichloroethane        | 71-55-6  | 100.0    | 2002                                | 2002                                         |
| 1,1,2-Trichloroethane        | 79-00-5  | 98.6     | 2000                                | 1972                                         |
| Trichloroethene              | 79-01-6  | 100.0    | 2003                                | 2003                                         |
| 1,2,3-Trichloropropane       | 96-18-4  | 97.5     | 2055*                               | 2004                                         |
| 1,2,4-Trimethylbenzene       | 95-63-6  | 98.2     | 2001                                | 1965                                         |
| 1,3,5-Trimethylbenzene       | 108-67-8 | 98.8     | 2001                                | 1977                                         |
| o-Xylene                     | 95-47-6  | 99.0     | 2000                                | 1980                                         |
| m-Xylene                     | 108-38-3 | 99.2     | 2002                                | 1986                                         |
| p-Xylene                     | 106-42-3 | 95.4     | 2097*                               | 2001                                         |

\* Weight compensated to 100% purity.

\*\* 47.8% cis isomer, 46.1% trans isomer

A product with a suffix (-1A, -2B, etc. or -01, -02, etc.) on its lot number has had its expiration date extended and is identical to the same lot number without the suffix.

<sup>2</sup> All weights are traceable through NIST, Test No. 684/289871-17

<sup>1</sup> Certified Analyte Concentration = Purity x Prepared Concentration.

The Uncertainty associated with the certified concentration reported on this certificate is  $\pm 2.4\%$ . This value is the combined expanded uncertainty and represents an estimated standard deviation equal to the positive square root of the total variation of the uncertainty of components. A normal distribution is assumed and a coverage factor of K=2 is chosen using approximately a 95% confidence level.

Labels and certificates follow U.S. Conventions in reporting numerical values: A comma (,) is used to separate units of one-thousand or greater. A period (.) is used as a decimal place marker.

The information on this certificate may not be reproduced without the express permission of the manufacturer. See reverse side for additional information

Certified By: 

Larry Decker, Organic QC Manager

**ID #:** 12797

Opened: \_\_\_\_\_

Volatile Organic Compounds - Liquids

**Expires:** 4/13/2023

Rec'd: 6/23/2020

Energy Laboratories Inc 1120 So. 27th Street  
Billings MT 59107

# Certificate of Analysis

**Product Name:** VOC Standard

**Product Number:** DWM-589N-1

**Lot Number:** 0006570990

**Lot Issue Date:** 17-Nov-2020

**Expiration Date:** 31-Dec-2023


**Description:**

This analytical reference material (RM) was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed below.

| Analyte                   | CAS#        | Analyte Lot | Concentration ± Uncertainty |
|---------------------------|-------------|-------------|-----------------------------|
| bromochloromethane        | 000074-97-5 | RM00009     | 2010 ± 10 µg/mL             |
| bromodichloromethane      | 000075-27-4 | RM12585     | 2009 ± 10 µg/mL             |
| bromoform                 | 000075-25-2 | RM13987     | 2010 ± 10 µg/mL             |
| carbon tetrachloride      | 000056-23-5 | RM07576     | 2010 ± 10 µg/mL             |
| chloroform                | 000067-66-3 | RM13988     | 2009 ± 10 µg/mL             |
| dibromochloromethane      | 000124-48-1 | RM14843     | 2009 ± 10 µg/mL             |
| dibromomethane            | 000074-95-3 | RM12878     | 2009 ± 10 µg/mL             |
| methylene chloride        | 000075-09-2 | RM11650     | 2009 ± 10 µg/mL             |
| 1,2-dibromoethane         | 000106-93-4 | RM00018     | 2010 ± 10 µg/mL             |
| 1,1-dichloroethane        | 000075-34-3 | RM16217     | 2006 ± 10 µg/mL             |
| 1,2-dichloroethane        | 000107-06-2 | RM04655     | 2005 ± 10 µg/mL             |
| 1,1-dichloroethene        | 000075-35-4 | RM14486     | 2010 ± 10 µg/mL             |
| cis-1,2-dichloroethene    | 000156-59-2 | RM15008     | 2007 ± 10 µg/mL             |
| trans-1,2-dichloroethene  | 000156-60-5 | RM07565     | 2008 ± 10 µg/mL             |
| 1,1,1,2-tetrachloroethane | 000630-20-6 | RM12632     | 2005 ± 10 µg/mL             |
| 1,1,2,2-tetrachloroethane | 000079-34-5 | RM02540     | 2009 ± 10 µg/mL             |
| tetrachloroethene         | 000127-18-4 | RM06491     | 2008 ± 10 µg/mL             |

# Certificate of Analysis

|                             |             |                    |                 |
|-----------------------------|-------------|--------------------|-----------------|
| <b>Product Number:</b>      | DWM-589N-1  | <b>Lot Number:</b> | 0006570990      |
| 1,1,1-trichloroethane       | 000071-55-6 | RM16539            | 2004 ± 10 µg/mL |
| 1,1,2-trichloroethane       | 000079-00-5 | RM01175            | 2009 ± 10 µg/mL |
| trichloroethene             | 000079-01-6 | RM14232            | 2009 ± 10 µg/mL |
| 1,2-dibromo-3-chloropropane | 000096-12-8 | RM13666            | 2009 ± 10 µg/mL |
| 1,2-dichloropropane         | 000078-87-5 | RM12821            | 2008 ± 10 µg/mL |
| 1,3-dichloropropane         | 000142-28-9 | RM02080            | 2008 ± 10 µg/mL |
| 2,2-dichloropropane         | 000594-20-7 | RM12927            | 2005 ± 10 µg/mL |
| 1,1-dichloropropene         | 000563-58-6 | RM16190            | 2010 ± 10 µg/mL |
| cis-1,3-dichloropropene     | 010061-01-5 | RM12891            | 2007 ± 10 µg/mL |
| trans-1,3-dichloropropene   | 010061-02-6 | RM12254            | 2006 ± 10 µg/mL |
| hexachlorobutadiene         | 000087-68-3 | RM09157            | 2005 ± 10 µg/mL |
| 1,2,3-trichloropropane      | 000096-18-4 | RM13082            | 2004 ± 10 µg/mL |
| benzene                     | 000071-43-2 | RM12931            | 2009 ± 10 µg/mL |
| n-butylbenzene              | 000104-51-8 | RM03651            | 2008 ± 10 µg/mL |
| sec-butylbenzene            | 000135-98-8 | RM10905            | 2005 ± 10 µg/mL |
| tert-butylbenzene           | 000098-06-6 | RM14040            | 2007 ± 10 µg/mL |
| ethylbenzene                | 000100-41-4 | RM12195            | 2006 ± 10 µg/mL |
| isopropylbenzene            | 000098-82-8 | RM00835            | 2009 ± 10 µg/mL |
| 4-isopropyltoluene          | 000099-87-6 | RM09747            | 2009 ± 10 µg/mL |
| naphthalene                 | 000091-20-3 | NT00970            | 2006 ± 10 µg/mL |
| n-propylbenzene             | 000103-65-1 | RM12785            | 2010 ± 10 µg/mL |
| styrene                     | 000100-42-5 | RM13393            | 2010 ± 10 µg/mL |



ISO 17034 Cert  
No. AR-1936

RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality Management System. Cert # 56 100 18560026

Page: 2 of 4

[www.agilent.com/quality/](http://www.agilent.com/quality/)  
CSD-QA-015.1



ISO 17025 Cert  
No. AT-1937



# Certificate of Analysis

**Product Number:** DWM-589N-1

**Lot Number:** 0006570990

|                        |             |         |                 |
|------------------------|-------------|---------|-----------------|
| toluene                | 000108-88-3 | RM06650 | 2008 ± 10 µg/mL |
| 1,2,4-trimethylbenzene | 000095-63-6 | RM06731 | 2002 ± 10 µg/mL |
| 1,3,5-trimethylbenzene | 000108-67-8 | RM12905 | 2009 ± 10 µg/mL |
| o-xylene               | 000095-47-6 | RM15639 | 2005 ± 10 µg/mL |
| m-xylene               | 000108-38-3 | RM15919 | 2006 ± 10 µg/mL |
| p-xylene               | 000106-42-3 | RM02647 | 2009 ± 10 µg/mL |
| bromobenzene           | 000108-86-1 | RM10227 | 2008 ± 10 µg/mL |
| chlorobenzene          | 000108-90-7 | RM01874 | 2008 ± 10 µg/mL |
| 2-chlorotoluene        | 000095-49-8 | RM13774 | 2007 ± 10 µg/mL |
| 4-chlorotoluene        | 000106-43-4 | RM11750 | 2009 ± 10 µg/mL |
| 1,2-dichlorobenzene    | 000095-50-1 | RM13636 | 2005 ± 10 µg/mL |
| 1,3-dichlorobenzene    | 000541-73-1 | NT00356 | 2009 ± 10 µg/mL |
| 1,4-dichlorobenzene    | 000106-46-7 | RM12826 | 2009 ± 10 µg/mL |
| 1,2,3-trichlorobenzene | 000087-61-6 | RM10193 | 2007 ± 10 µg/mL |
| 1,2,4-trichlorobenzene | 000120-82-1 | RM09454 | 2009 ± 10 µg/mL |

**Matrix:** methanol (methyl alcohol)

**Storage Conditions:** Store Frozen (-25° to -10°C).

### Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCCL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

### Homogeneity:

This RM was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.



ISO 17034 Cert  
No. AR-1936

RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality Management System. Cert # 56 100 18560026

Page: 3 of 4

[www.agilent.com/quality/](http://www.agilent.com/quality/)  
CSD-QA-015.1



ISO 17025 Cert  
No. AT-1937



# Certificate of Analysis

Product Number: DWM-589N-1

Lot Number: 0006570990

## Intended Use:

This RM is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

## Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

## Hazards:

Refer to the Safety Data Sheet on [www.agilent.com](http://www.agilent.com) for information regarding this RM.


## Expiration of Certification:

The certification of this RM is valid until the expiration date specified above, provided the RM is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the RM is damaged, contaminated, or otherwise modified.

## Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:



Monica Bourgeois  
QMS Representative



ISO 17034 Cert  
No. AR-1936

RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality Management System. Cert # 56 100 18560026

Page: 4 of 4

[www.agilent.com/quality/](http://www.agilent.com/quality/)  
CSD-QA-015.1



ISO 17025 Cert  
No. AT-1937

# Certificate of Analysis

**Product Name:** Methyl tert-Butyl Ether Standard**Product Number:** STS-440-1**Lot Number:** 0006555762**Lot Issue Date:** 19-Aug-2020**Expiration Date:** 31-Aug-2022**Description:**

This analytical reference material (RM) was manufactured and verified in accordance with an ISO 9001 registered quality system, and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed below.

**Analyte****CAS#****Analyte Lot****Concentration ± Uncertainty**

tert-butylmethyl ether

001634-04-4

RM06568

2006 ± 10 µg/mL

**Matrix:** methanol (methyl alcohol)**Storage Conditions:** Store Frozen (-25° to -10°C).**Traceability:**

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

**Homogeneity:**

This RM was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

**Intended Use:**

This RM is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

**Instructions for Use:**

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

**Hazards:**


Refer to the Safety Data Sheet on [www.agilent.com](http://www.agilent.com) for information regarding this RM.

**Expiration of Certification:**

The certification of this RM is valid until the expiration date specified above, provided the RM is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the RM is damaged, contaminated, or otherwise modified.

**Maintenance of Certification:**

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

**Sample lot approver:**

Monica Bourgeois

QMS Representative

ISO 17034 Cert  
No. AR-1936RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality  
Management System. Cert # 56 100 18560026

Page: 1 of 1

[www.agilent.com/quality/](http://www.agilent.com/quality/)  
CSD-QA-015.1ISO 17025 Cert  
No. AT-1937

# CERTIFICATE OF ANALYSIS

**Catalog No:** S-078-10X

**Description:** MtBE

**Lot:** 220051182

**Solvent:** Methanol

**Hazards:** Refer to SDS for complete safety information

**Date Certified:** May 18, 2020

**Expiration:** May 18, 2030

**Sample Size:** 1 mL

**Components:** 1

**Storage Condition:** Ambient (>5 °C)



Signal Word: **Danger**

**Certified Reference Material**



| Component | CAS #     | Purity %<br>(GC/MS) | Prepared<br>Concentration <sup>2</sup><br>(µg/mL) | Certified Analyte<br>Concentration <sup>1</sup><br>(µg/mL) |
|-----------|-----------|---------------------|---------------------------------------------------|------------------------------------------------------------|
| MTBE      | 1634-04-4 | 100.0               | 2002                                              | 2002                                                       |

**ID #:** 13920

Opened: \_\_\_\_\_

MTBE

**Expires:** 5/18/2030

Rec'd: 6/7/2021

Eneray Laboratories Inc 1120 So. 27th Street  
Billings MT 59107

A product with a suffix (-1A, -2B, etc. or -01, -02, etc.) on its lot number has had its expiration date extended and is identical to the same lot number without the suffix.

<sup>2</sup> All weights are traceable through NIST, Test No. 684/289871-17

<sup>1</sup> Certified Analyte Concentration = Purity x Prepared Concentration.

The Uncertainty associated with the certified concentration reported on this certificate is  $\pm 2.4\%$ . This value is the combined expanded uncertainty and represents an estimated standard deviation equal to the positive square root of the total variation of the uncertainty of components. A normal distribution is assumed and a coverage factor of K=2 is chosen using approximately a 95% confidence level.

Labels and certificates follow U.S. Conventions in reporting numerical values: A comma (,) is used to separate units of one-thousand or greater. A period (.) is used as a decimal place marker.

The information on this certificate may not be reproduced without the express permission of the manufacturer. See reverse side for additional information

Hazard Information: Please refer to the SDS for information regarding the hazards associated with using this material.

This product was prepared according to in-house procedures and is guaranteed to be homogeneous.

Certified By: \_\_\_\_\_

Larry Decker, Organic QC Manager

## CERTIFICATE OF ANALYSIS

### Volatile Organics High Concentration Mixture #6

CONCENTRATION 2000ug/ml in Methanol  
CATALOG NUMBER M-VOHC6M5-1ML  
LOT NUMBER 11882100  
DATE CERTIFIED 05/25/21  
EXPIRATION DATE 02/28/22  
STORAGE Store at room temperature (20 - 25 °C).  
HANDLING See Safety Data Sheet  
INTENDED USE For laboratory use only.  
ISO 17034:2016 CERTIFIED [ ]

ID #: 14142

Opened:

Volatile Organics High Concentration Mixture

Expires: 2/28/2022

Rec'd: 8/3/2021

Energx Laboratories Inc 1120 So. 27th Street  
Billings MT 59107

| ID      | Analyte                 | CAS     | Weight Analyte (mg) | Lot      | Purity | Certified Concentration (ug/mL) |
|---------|-------------------------|---------|---------------------|----------|--------|---------------------------------|
| N-11446 | Chloroethane            | 75-00-3 | 96.300              | 00001728 | 100.0  | 2006.3                          |
| N-11665 | Dichlorodifluoromethane | 75-71-8 | 96.610              | 00001729 | 100.0  | 2012.7                          |
| N-12417 | Methyl bromide          | 74-83-9 | 96.910              | 00024694 | 100.0  | 2019.0                          |
| N-12421 | Methyl chloride         | 74-87-3 | 96.150              | 00001731 | 100.0  | 2003.1                          |
| N-13655 | Trichlorofluoromethane  | 75-69-4 | 96.300              | 00027239 | 99.4   | 1994.2                          |
| N-13748 | Vinyl chloride          | 75-01-4 | 96.150              | 00019298 | 100.0  | 2003.1                          |

#### Analytical Test


#### Value

CONCENTRATION (GC/MSD)

VERIFIED

COA Form  
Revision 3 (3/2015)

Print Date: 07/28/21



# CHEM SERVICE INC

660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599  
1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729  
[info@chemservice.com](mailto:info@chemservice.com) • [www.chemservice.com](http://www.chemservice.com)

## Instructions for Use:

Shake mixture prior to use. If particles are present, sonicate for homogeneity. If sample is diluted to lower concentrations, Class A volumetric glassware must be used.

Minimum Sample Size- 0.2 uL for Direct Injection.

Chem Service Inc. guarantees the expanded uncertainty of the above analytes to be +/- 2.0% of the certified concentrations based on gravimetric preparation. The test results published in this report were obtained using equipment capable of producing results that are traceable to NIST and through NIST to the International System of Units (SI). The reported expanded uncertainty of measurement is stated as the combined standard uncertainty of measurement multiplied by the coverage factor k (k=2) such that the coverage probability corresponds to approximately 95%. For certified reference materials, homogeneity and thermal stability testing are available upon request.

Certified By:

*Mary Beth O'Donnell*


Mary Beth O'Donnell  
CSM/TC



## CERTIFICATE OF ANALYSIS

### Analysis Method:

Catalog Number: M-VOHC6M5-1ML  
Description: Volatile Organics High Concentration Mixture #6  
Lot Number: 11882100  
Expiration Date: 02/28/22

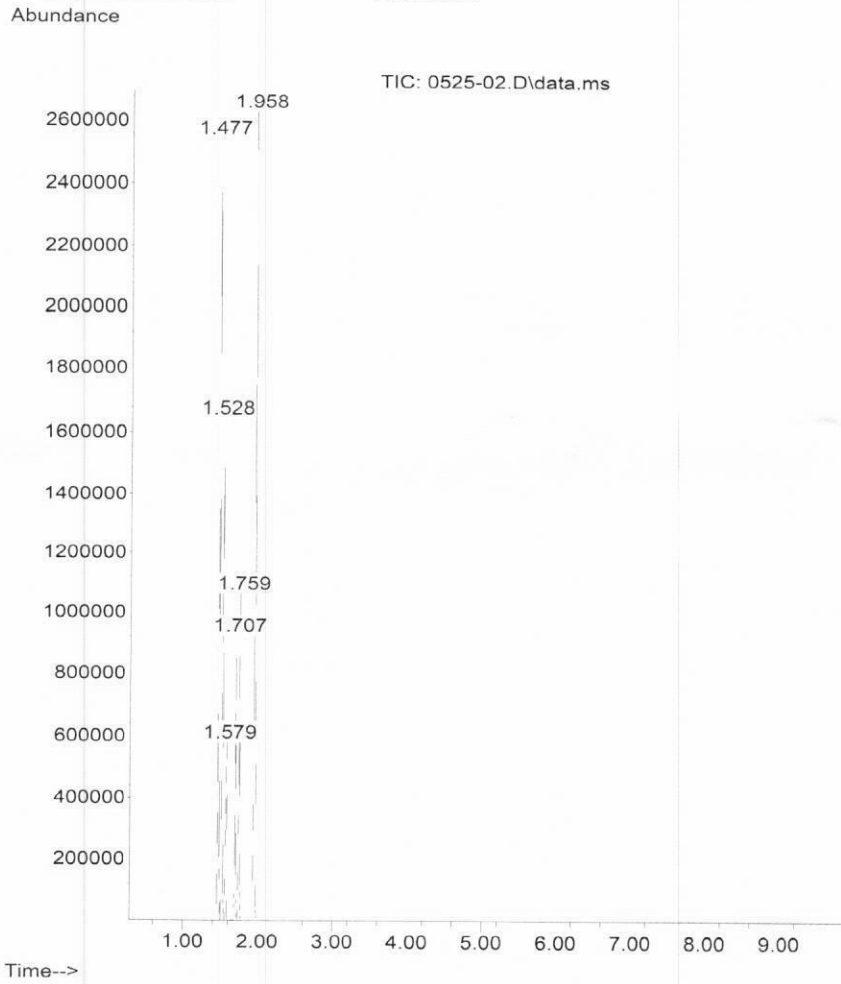



# Certificate of Analysis

ID #: 14251

Opened: \_\_\_\_\_

Internal Standard

Expires: 12/31/2022

Rec'd: 9/8/2021

Energy Laboratories Inc 1120 So. 27th Street  
Billings MT 59107

Product Name: Internal Standard

Product Number: STM-520-1

Lot Issue Date: 05-Jan-2021

Lot Number: 0006582580

Expiration Date: 31-Dec-2022

## Description:

This analytical reference material (RM) was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed below.

| Analyte                | CAS#        | Analyte Lot | Concentration ± Uncertainty |
|------------------------|-------------|-------------|-----------------------------|
| chlorobenzene-d5       | 003114-55-4 | RM12274     | 2501 ± 13 µg/mL             |
| 1,4-dichlorobenzene-d4 | 003855-82-1 | RM12517     | 2501 ± 13 µg/mL             |
| fluorobenzene          | 000462-06-6 | RM13378     | 2512 ± 13 µg/mL             |

Matrix: methanol (methyl alcohol)

Storage Conditions: Store Frozen (-25° to -10°C).

## Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCCL Z540.3, ISO 9001, ISO 17025 and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

## Homogeneity:

This RM was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

## Intended Use:

This RM is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

## Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

## Hazards:

Refer to the Safety Data Sheet on [www.agilent.com](http://www.agilent.com) for information regarding this RM.



ISO 17034  
REFERENCE MATERIAL  
PRODUCER  
ISO 17034 Cert  
No. AR-1936

RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality  
Management System. Cert # 56 100 18560026

Page: 1 of 2

[www.agilent.com/quality/](http://www.agilent.com/quality/)  
CSD-QA-015.1



ISO 17025 Cert  
No. AT-1937



# Certificate of Analysis

**Product Number:** STM-520-1

**Lot Number:** 0006582580

**Expiration of Certification:**

The certification of this RM is valid until the expiration date specified above, provided the RM is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the RM is damaged, contaminated, or otherwise modified.

**Maintenance of Certification:**

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

**Sample lot approver:**

Monica Bourgeois  
QMS Representative



ISO 17034 Cert  
No. AR-1936

RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality Management System. Cert # 56 100 18560026

Page: 2 of 2

[www.agilent.com/quality/](http://www.agilent.com/quality/)  
CSD-QA-015.1



ISO 17025 Cert  
No. AT-1937



# CERTIFICATE OF ANALYSIS

**Catalog No:** M-8260A-B-SS-10X  
**Description:** Surrogate Standard Mix  
**Lot:** 219041458

**Solvent:** Methanol

**Hazards:** Refer to SDS for complete safety information

**Date Certified:** Apr 18, 2019

**Expiration:** Apr 18, 2029

**Sample Size:** 1 mL

**Components:** 4

**Storage Condition:** Ambient (>5 °C)



Signal Word: Danger

## Certified Reference Material



| Component             | CAS #      | Purity %<br>(GC/MS) | Prepared<br>Concentration <sup>2</sup><br>(µg/mL) | Certified Analyte<br>Concentration <sup>1</sup><br>(µg/mL) |
|-----------------------|------------|---------------------|---------------------------------------------------|------------------------------------------------------------|
| p-Bromofluorobenzene  | 460-00-4   | 99.9                | 2004                                              | 2002                                                       |
| Dibromofluoromethane  | 1868-53-7  | 99.8                | 2005                                              | 2001                                                       |
| 1,2-Dichloroethane-d4 | 17060-07-0 | 100.0               | 2001                                              | 2001                                                       |
| Toluene-d8            | 2037-26-5  | 100.0               | 2000                                              | 2000                                                       |

ID #: 14269

Opened: \_\_\_\_\_

Surrogate Standard Mix

**Expires: 4/18/2029**

Rec'd: 9/14/2021

Energy Laboratories Inc 1120 So. 27th Street  
Billings MT 59107

A product with a suffix (-1A, -2B, etc. or -01, -02, etc.) on its lot number has had its expiration date extended and is identical to the same lot number without the suffix.

<sup>2</sup> All weights are traceable through NIST, Test No. 684/289871-17

<sup>1</sup> Certified Analyte Concentration = Purity x Prepared Concentration.

The Uncertainty associated with the certified concentration reported on this certificate is  $\pm 2.4\%$ . This value is the combined expanded uncertainty and represents an estimated standard deviation equal to the positive square root of the total variation of the uncertainty of components. A normal distribution is assumed and a coverage factor of K=2 is chosen using approximately a 95% confidence level.

Labels and certificates follow U.S. Conventions in reporting numerical values: A comma (,) is used to separate units of one-thousand or greater. A period (.) is used as a decimal place marker.



The information on this certificate may not be reproduced without the express permission of the manufacturer. See reverse side for additional information

Hazard Information: Please refer to the SDS for information regarding the hazards associated with using this material.

This product was prepared according to in-house procedures and is guaranteed to be homogeneous.

Certified By: \_\_\_\_\_

Larry Decker, Organic QC Manager



**CERTIFIED WEIGHT REPORT**

**Part Number:** 30058  
**Lot Number:** 080321  
**Description:** EPA Method 502/524 - Volatile Gases Mix #1

**Expiration Date:** 080324

**Recommended Storage:** Freezer (0 °C)

**Nominal Concentration (µg/mL):** 2000

**NIST Test ID#:** 6UTB

**Solvent:** Methanol  
**Lot#:** EA783-US

Weight(s) shown below were combined and diluted to (mL):  
500.0 0.058 Balance Uncertainty  
0.058 Flask Uncertainty


|                |                 |        |
|----------------|-----------------|--------|
|                |                 | 080321 |
| Formulated By: | Mario Luis      | DATE   |
|                |                 | 080321 |
| Reviewed By:   | Pedro L. Rentas | DATE   |

| Compound                   | RM# | Lot Number | Nominal Conc (µg/mL) | Purity (%) | Uncertainty Purity (%) | Target Weight (g) | Actual Weight (g) | Actual Conc(µg/mL) | Expanded Uncertainty (+/-) (µg/mL) | SDS Information (Solvent Safety Info. On Attached pg.) |                           |                   |
|----------------------------|-----|------------|----------------------|------------|------------------------|-------------------|-------------------|--------------------|------------------------------------|--------------------------------------------------------|---------------------------|-------------------|
|                            |     |            |                      |            |                        |                   |                   |                    |                                    | CAS#                                                   | OSHA PEL (TWA)            | LD50              |
| 1. Bromomethane            | 50  | 01611JX    | 2000                 | 99.5       | 0.2                    | 1.00508           | 1.0098            | 2009.4             | 8.1                                | 74-83-9                                                | 5 ppm (20mg/m3/8H) (skin) | ori-rat 214mg/kg  |
| 2. Chloroethane            | 72  | 062617     | 2000                 | 99         | 0.2                    | 1.01016           | 1.0146            | 2008.8             | 8.1                                | 75-00-3                                                | 1000 ppm (2600mg/m3/8H)   | N/A               |
| 3. Chloromethane           | 79  | 06908MS    | 2000                 | 99.5       | 0.2                    | 1.00508           | 1.0154            | 2020.5             | 8.1                                | 74-87-3                                                | 100 ppm                   | ori-rat 1800mg/kg |
| 4. Dichlorodifluoromethane | 134 | 92-0487    | 2000                 | 99         | 0.2                    | 1.01016           | 1.0224            | 2024.2             | 8.2                                | 75-71-8                                                | 1000 ppm (4950mg/m3/8H)   | N/A               |
| 5. Trichlorofluoromethane  | 294 | 01823MW    | 2000                 | 99         | 0.2                    | 1.01016           | 1.0110            | 2001.7             | 8.1                                | 75-69-4                                                | 1000 ppm (5600mg/m3/8H)   | ipr-mus 1743mg/kg |
| 6. Vinyl chloride          | 305 | 04854EA    | 2000                 | 99.5       | 0.2                    | 1.00508           | 1.0071            | 2004.0             | 8.1                                | 75-01-4                                                | N/A                       | N/A               |

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

**Comments**

GC15-M9 Analysis by Melissa Stonier  
Column ID SPB-Vocool 105 meter X 0.53mm X 3.0µm film thickness  
Flow rates: Total flow=150mL/min., Helium (carrier)=10mL/min., Helium(make-up)=40mL/min., Hydrogen(make-up)=100mL/min.  
Oven Profile: Temp. 1=35°C (Time 1=9 min.), Temp 2=200°C (Time 2=1 min.), Rate = 33°C/min., Total run time=15 min. Injector temp.=200°C, FID Temp.=200°C.  
ELCD Signal = Edaq Channel 1 PID Signal = Edaq Channel 2  
Standard injection = 0.5µL, Range=3 Purge Valve = 0 min.



| Peak No. | Analyte                 | ELCD RT (min.) |
|----------|-------------------------|----------------|
| 1        | Dichlorodifluoromethane | 4.67           |
| 2        | Chloromethane           | 5.28           |
| 3        | Vinyl chloride          | 5.56           |
| 4        | Bromomethane            | 6.75           |
| 5        | Chloroethane            | 6.99           |
| 6        | Trichlorofluoromethane  | 7.72           |

**ID #: 14285**

Opened: \_\_\_\_\_  
EPA Method 502-524 - Volatile Gases Mix #1  
**Expires: 8/3/2024**  
Rec'd: 9/17/2021  
Energy Laboratories Inc 1120 So. 27th Street  
Billings MT 59107

660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599  
1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729  
[info@chemservice.com](mailto:info@chemservice.com) • [www.chemservice.com](http://www.chemservice.com)

ID #: 14443

Opened: \_\_\_\_\_

TCL Ketone Mix

Expires: 6/30/2023

Rec'd: 10/26/2021

Energy Laboratories Inc 1120 So. 27th Street  
Billings MT 59107

## CERTIFICATE OF ANALYSIS

### TCL Ketones Mixture

CONCENTRATION 2000ug/ml in Methanol:Water (90:10)  
CATALOG NUMBER M-TCL1AN5-1ML  
LOT NUMBER 10251200  
DATE CERTIFIED 06/16/20  
EXPIRATION DATE 06/30/23  
STORAGE Freezer storage (-20 - -25 °C)  
HANDLING See Safety Data Sheet  
INTENDED USE For laboratory use only.  
ISO 17034:2016 CERTIFIED [ ]

| ID      | Analyte              | CAS      | Weight Analyte (mg) | Lot      | Purity | Certified Concentration (ug/mL) |
|---------|----------------------|----------|---------------------|----------|--------|---------------------------------|
| N-11014 | Acetone              | 67-64-1  | 203.300             | 00026182 | 98.7   | 2006.6                          |
| N-10297 | 2-Butanone           | 78-93-3  | 202.800             | 00027454 | 99.5   | 2017.9                          |
| N-10369 | 2-Hexanone           | 591-78-6 | 202.600             | 00025720 | 99.5   | 2015.9                          |
| N-10844 | 4-Methyl-2-pentanone | 108-10-1 | 204.700             | 6403300  | 99.5   | 2036.8                          |

| Analytical Test        | Value    |
|------------------------|----------|
| CONCENTRATION (GC/FID) | VERIFIED |

Chem Service, Inc. is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015.



COA Form  
Revision 3 (3/2015)

Print Date: 10/22/21

660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599  
1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729  
[info@chemservice.com](mailto:info@chemservice.com) • [www.chemservice.com](http://www.chemservice.com)

**Instructions for Use:**

Shake mixture prior to use. If particles are present, sonicate for homogeneity. If sample is diluted to lower concentrations, Class A volumetric glassware must be used.

Minimum Sample Size- 0.2 uL for Direct Injection.

Chem Service Inc. guarantees the expanded uncertainty of the above analytes to be +/- 2.0% of the certified concentrations based on gravimetric preparation. The test results published in this report were obtained using equipment capable of producing results that are traceable to NIST and through NIST to the International System of Units (SI). The reported expanded uncertainty of measurement is stated as the combined standard uncertainty of measurement multiplied by the coverage factor k (k=2) such that the coverage probability corresponds to approximately 95%. For certified reference materials, homogeneity and thermal stability testing are available upon request.

**Certified By:**

*Mary Beth O'Donnell*

Mary Beth O'Donnell  
CSM/TC

Chem Service, Inc. is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015.




660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599  
 1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729  
[info@chemservice.com](mailto:info@chemservice.com) • [www.chemservice.com](http://www.chemservice.com)

## CERTIFICATE OF ANALYSIS

Gas Chromatography / Flame Ionization Detector (GC/FID)

**Data file:** C:\CHEM321\DATA\2020 DATA\0620M-TCL1AN5.D  
**Sample name:** M-TCL1AN5  
**Acq. method:** N-14278.M  
**Instrument:** GC3  
**Injection date:** 6/16/2020 2:52:35 PM  
**Column name:** RTX-5MS (30m x 0.25mm x 0.5µm)  
**# Of Injections:** 1  
**Injection Vol:** 1.000  
**Location:** 202

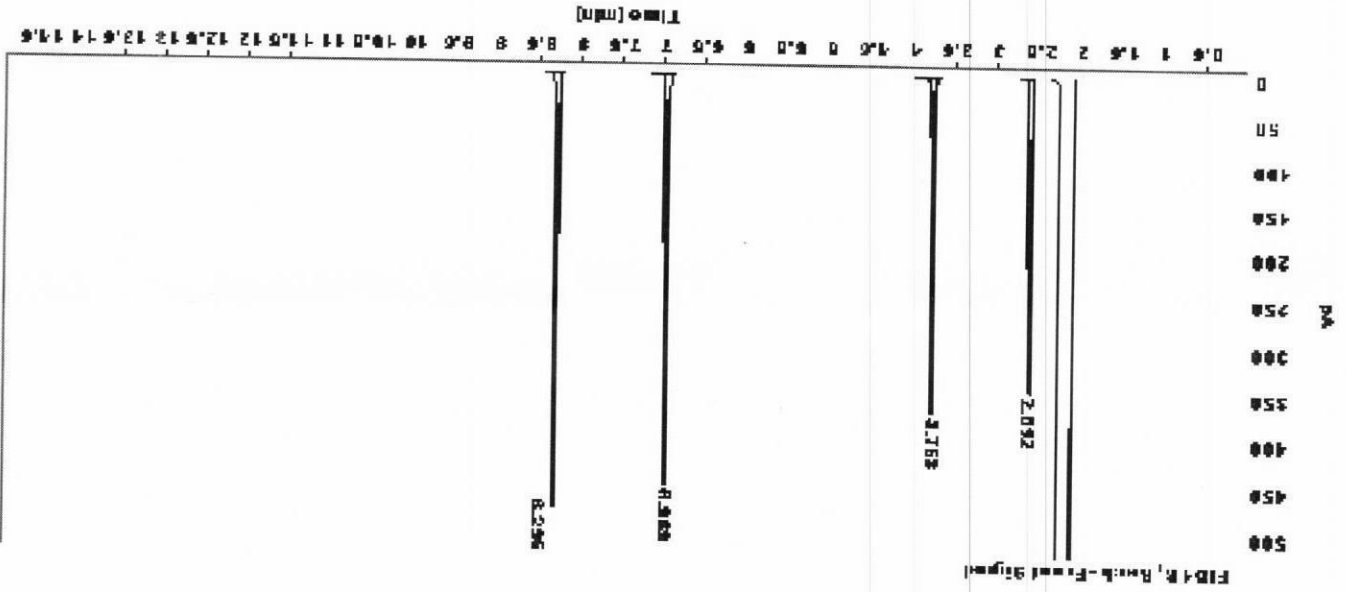

FID1 B, Back - Front signal

Signal: FID1 B, Back - Front signal

| RT [min] | Type | Width [min] | Area     | Height   | Area%     |
|----------|------|-------------|----------|----------|-----------|
| 2.592    | BB   | 0.0277      | 580.2505 | 343.4986 | 18.4855   |
| 3.763    | BB   | 0.0323      | 735.4804 | 387.8491 | 23.4054   |
| 6.969    | BB   | 0.0326      | 904.3389 | 447.8770 | 28.7791   |
| 8.295    | BB   | 0.0307      | 822.2798 | 474.3798 | 29.3500   |
| Sum      |      |             |          |          | 3142.3497 |

Chem Service, Inc is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015.



# CERTIFICATE OF ANALYSIS

**Catalog No:** CLP-022K-10X  
**Description:** TCL Ketone Mix  
**Lot:** 221101480  
**Solvent:** Methanol  
**Hazards:** Refer to SDS for complete safety information

**Date Certified:** Oct 26, 2021  
**Expiration:** Nov 26, 2022  
**Sample Size:** 1 mL  
**Components:** 4  
**Storage Condition:** Freeze (<-10 °C)



**Certified Reference Material**



| Component            | CAS #    | Purity % | Prepared Concentration <sup>2</sup> | Certified Analyte Concentration <sup>1</sup> |
|----------------------|----------|----------|-------------------------------------|----------------------------------------------|
|                      |          | (GC/MS)  | (µg/mL)                             | (µg/mL)                                      |
| Acetone              | 67-64-1  | 100.0    | 2004                                | 2004                                         |
| 2-Butanone           | 78-93-3  | 100.0    | 2004                                | 2004                                         |
| 2-Hexanone           | 591-78-6 | 98.7     | 2004                                | 1978                                         |
| 4-Methyl-2-pentanone | 108-10-1 | 100.0    | 2004                                | 2004                                         |

**ID #: 14567**

Opened: \_\_\_\_\_  
TCL Ketones Mixture  
**Expires: 11/26/2022**  
Rec'd: 11/30/2021  
Energy Laboratories Inc 1120 So. 27th Street  
Billings MT 59107

This Certified Reference Material was verified in accordance with ISO/IEC 17025

A product with a suffix (-1A, -2B, etc. or -01, -02, etc.) on its lot number has had its expiration date extended and is identical to the same lot number without the suffix.

<sup>2</sup> All weights are traceable through NIST, Test No. 684/289871-17

<sup>1</sup> Certified Analyte Concentration = Purity x Prepared Concentration.

The Uncertainty associated with the certified concentration reported on this certificate is ±2.4%. This value is the combined expanded uncertainty and represents an estimated standard deviation equal to the positive square root of the total variation of the uncertainty of components. A normal distribution is assumed and a coverage factor of K=2 is chosen using approximately a 95% confidence level.

Labels and certificates follow U.S. Conventions in reporting numerical values: A comma (,) is used to separate units of one-thousand or greater. A period (.) is used as a decimal place marker.

The information on this certificate may not be reproduced without the express permission of the manufacturer. See reverse side for additional information

Hazard Information: Please refer to the SDS for information regarding the hazards associated with using this material.

This product was prepared according to in-house procedures and is guaranteed to be homogeneous.

Certified By: \_\_\_\_\_

Larry Decker, Organic QC Manager

# CERTIFICATE OF ANALYSIS

**Catalog No:** CLP-022K-10X  
**Description:** TCL Ketone Mix  
**Lot:** 221101480  
**Solvent:** Methanol

**Date Certified:** Oct 26, 2021  
**Expiration:** Nov 26, 2022  
**Sample Size:** 1 mL  
**Components:** 4

## T-Test

AccuStandard, Inc.  
Statistical Report for CLP (SOW 1391)  
26-Oct-2021

QR-QC-003 rev. 1/16

| RT Component                         | CLP-022K-10X<br>221101480 |        |        |        |      |         |       | CLP-022K-10X<br>221041075 |        |        |        |      |         |       | NOTES:     |       |                                 |      |           |                                 |     |
|--------------------------------------|---------------------------|--------|--------|--------|------|---------|-------|---------------------------|--------|--------|--------|------|---------|-------|------------|-------|---------------------------------|------|-----------|---------------------------------|-----|
|                                      | Run #1                    | Run #2 | Run #3 | Run #4 | Mean | Std Dev | % RSD | Run #1                    | Run #2 | Run #3 | Run #4 | Mean | Std Dev | % RSD | t.025 test | CI    | Component                       | CI   | # of Runs | 10 % error check of Conc. means |     |
| 3.74 Acetone (67-64-1)               | 1925                      | 1881   | 1854   | 1803   | 1866 | 51.05   | 2.74% | 1751                      | 1712   | 1730   | 1764   | 1764 | 22.43   | 1.29% | 4.36       | 119.2 | Acetone (67-64-1)               | 56   | 4         | 2000                            | 7 % |
| 5.77 2-Butanone (78-93-3)            | 2275                      | 2223   | 2237   | 2149   | 2221 | 52.79   | 2.38% | 2157                      | 2103   | 2145   | 2177   | 2146 | 31.26   | 1.45% | 2.46       | 58.5  | 2-Butanone (78-93-3)            | 35.9 | 4         | 2000                            | 9 % |
| 8.34 4-Methyl-2-pentanone (108-10-1) | 3373                      | 3302   | 3408   | 3225   | 3327 | 81.05   | 2.44% | 3349                      | 3240   | 3296   | 3415   | 3325 | 74.70   | 2.25% | 0.04       | 0.9   | 4-Methyl-2-pentanone (108-10-1) | 0.8  | 4         | 2000                            | 0 % |
| 9.13 2-Hexanone (98-178-6)           | 3260                      | 3199   | 3332   | 3118   | 3227 | 90.88   | 2.62% | 3186                      | 3072   | 3120   | 3239   | 3154 | 73.32   | 2.32% | 1.25       | 35.2  | 2-Hexanone (98-178-6)           | 29.1 | 4         | 2000                            | 2 % |


# CERTIFICATE OF ANALYSIS

**Catalog No:** CLP-022K-10X  
**Description:** TCL Ketone Mix  
**Lot:** 221101480  
**Solvent:** Methanol

**Date Certified:** Oct 26, 2021  
**Expiration:** Nov 26, 2022  
**Sample Size:** 1 mL  
**Components:** 4

## Chromatogram

File : Q:\GCMS-06 Minimal\DATA\102521\13- 221101480 KM.D  
Operator : Organic QC Lab  
Acquired : 25 Oct 2021 21:00 using AcqMethod VOC-Split100.M  
Instrument : GCMS 6  
Sample Name : CLP-022K-10X (221101480)  
Misc Info : TCL Ketone Mix @ 2000 ug/mL in MeOH  
Vial Number : 34



Column: DB-624 UI, 30m x 0.25mm ID x 1.4µm  
Oven Program: 35°C (hold 5min), 11°C/min to 60°C, 22°C/min to 230°C (hold 4min)  
GC Parameters: Split 100:1, 1µl inj.; GC/MS; injector temp 240°C

