

# Energy Laboratories Inc

# ANALYTICAL RUN Summary

13-Jan-22

Run ID GCFID-HP5-B\_220111A

<b>Run Start Date:</b>	1/11/2022
<b>Analyst:</b>	Ann Nebel
<b>Ical:</b>	
<b>Column ID:</b>	
<b>Comments:</b>	ICAL- SW8015C_DRO220111JA.CAL

Std ID	Std Name	Std Amount	Std Units	Samp Amount	Samp Units	SampType	Expiration Date
DRO211012B	#2 Diesel in Acetone 150,000 ug/mL					ICV	11/5/2023
DRO211101A	OTP-4000 ug/mL DCM					OTP-CAL	9/30/2024
DRO211214C	Diesel Fuel #2 50,000 ug/mL in DCM					CCV-CAL	4/30/2023
DRO220102D	ALASKA MARKER-200ug/mL					MARKER	5/31/2022

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976981	CCV_0111HP50	HC-8015-DRO-	CCV		1/11/2022 8:59:2	1	R373149		0	0						
<b>Analyte</b>		<b>T</b>	<b>Units</b>	<b>RAW</b>	<b>Final</b>	<b>Text</b>	<b>Spike</b>	<b>SPKref</b>	<b>RPDref</b>	<b>MDL</b>	<b>PQL</b>	<b>UQL</b>	<b>%REC</b>	<b>LOW</b>	<b>HIGH</b>	<b>%RPD</b> <b>Q</b>
Total Extractable Hydrocarbons	A	mg/L		3.205893			15	0	0	0.0749	0.3	50	21%	80	120	0% S
o-Terphenyl	S	mg/L		0.1968894			0.2	0	0	0.000429	0.002	0	98%	80	120	0%

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976982	CCV_0111HP50	HC-8015-DRO-	CAL1		1/11/2022 10:25:	1	R373149		0	0						
<b>Analyte</b>		<b>T</b>	<b>Units</b>	<b>RAW</b>	<b>Final</b>	<b>Text</b>	<b>Spike</b>	<b>SPKref</b>	<b>RPDref</b>	<b>MDL</b>	<b>PQL</b>	<b>UQL</b>	<b>%REC</b>	<b>LOW</b>	<b>HIGH</b>	<b>%RPD</b> <b>Q</b>
o-Terphenyl	S	mg/L		0.00201677			0.002	0	0	0.000429	0.002	0	101%	80	120	0%

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976983	CCV_0111HP50	HC-8015-DRO-	CAL2		1/11/2022 11:08:	1	R373149		0	0						
<b>Analyte</b>		<b>T</b>	<b>Units</b>	<b>RAW</b>	<b>Final</b>	<b>Text</b>	<b>Spike</b>	<b>SPKref</b>	<b>RPDref</b>	<b>MDL</b>	<b>PQL</b>	<b>UQL</b>	<b>%REC</b>	<b>LOW</b>	<b>HIGH</b>	<b>%RPD</b> <b>Q</b>
o-Terphenyl	S	mg/L		0.0489019			0.05	0	0	0.000429	0.002	0	98%	80	120	0%

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976984	CCV_0111HP50	HC-8015-DRO-	CAL3		1/11/2022 11:51:	1	R373149		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
o-Terphenyl	S	mg/L		0.2047389		0.2	0	0	0.000429	0.002	0	102%	80	120	0%	
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976985	CCV_0111HP50	HC-8015-DRO-	CAL4		1/11/2022 12:34:	1	R373149		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
o-Terphenyl	S	mg/L		0.4884362		0.5	0	0	0.000429	0.002	0	98%	80	120	0%	
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976986	CCV_0111HP50	HC-8015-DRO-	CAL5		1/11/2022 1:17:0	1	R373149		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
o-Terphenyl	S	mg/L		1.013008		1	0	0	0.000429	0.002	0	101%	80	120	0%	
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976987	CCV_0111HP50	HC-8015-DRO-	CAL1		1/11/2022 1:59:5	1	R373149		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Total Extractable Hydrocarbons	A	mg/L		0.1635249		0.15	0	0	0.0749	0.3	50	109%	80	120	0%	
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976989	CCV_0111HP51	HC-8015-DRO-	CAL2		1/11/2022 2:42:3	1	R373149		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Total Extractable Hydrocarbons	A	mg/L		3.698293		3.75	0	0	0.0749	0.3	50	99%	80	120	0%	
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976990	CCV_0111HP51	HC-8015-DRO-	CAL3		1/11/2022 3:25:2	1	R373149		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Total Extractable Hydrocarbons	A	mg/L		14.75864		15	0	0	0.0749	0.3	50	98%	80	120	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976991	CCV_0111HP51	HC-8015-DRO-	CAL4		1/11/2022 4:08:0	1	R373149		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Total Extractable Hydrocarbons	A	mg/L		36.29137		37.5	0	0	0.0749	0.3	50	97%	80	120	0%	
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976992	CCV_0111HP51	HC-8015-DRO-	CAL5		1/11/2022 4:51:0	1	R373149		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Total Extractable Hydrocarbons	A	mg/L		48.59718		50	0	0	0.0749	0.3	50	97%	80	120	0%	
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14976993	CCV_0111HP51	HC-8015-DRO-	ICV		1/11/2022 5:34:2	1	R373149		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Total Extractable Hydrocarbons	A	mg/L		14.05379		15	0	0	0.0749	0.3	50	94%	80	120	0%	

Write Sequence	Data File	Sample Name	Method	Weight	Dil Factor	Amt Inj.	IS	Cal ID
	G:\org\HP5\DAT\HP5011122_b\0111HP5.01r	DCM-Baseline Check-V01	G:\Org\HP5\Methods\DR_8015-IC-LEXP.met	1	1	1	1	0
	G:\org\HP5\DAT\HP5011122_b\0111HP5.02r	CCV_0111HP502r, DRO ;0111HP5 , DRO220102D	G:\Org\HP5\Methods\DC_8015-JA-L%.met	1	1	1	1	0
	G:\org\HP5\DAT\HP5011122_b\0111HP5.03r	DCM-Baseline Check-V03	G:\Org\HP5\Methods\DR_8015-IC-LEXP.met	1	1	1	1	0
	G:\org\HP5\DAT\HP5011122_b\0111HP5.04r	CCV_0111HP504r, CAL1 ;0111HP5 , 2 ug per mL OTP (10 uL of Cal3 + 990 uL DCM(14647)	G:\Org\HP5\Methods\DS_8015-JA-L#.met	1	1	1	1	0
	G:\org\HP5\DAT\HP5011122_b\0111HP5.05r	CCV_0111HP505r, CAL2 ;0111HP5 , 50 ug per mL OTP (100 uL Cal4 + 900 uL of DCM(14647)	G:\Org\HP5\Methods\DS_8015-JA-L#.met	1	1	1	1	0
	G:\org\HP5\DAT\HP5011122_b\0111HP5.06r	CCV_0111HP506r, CAL3 ;0111HP5 , 200 ug per mL OTP (100uL of Cal5 + 400 uL DCM(14647)	G:\Org\HP5\Methods\DS_8015-JA-L#.met	1	1	1	1	0
	G:\org\HP5\DAT\HP5011122_b\0111HP5.07r	CCV_0111HP507r, CAL4 ;0111HP5 , 500 ug per mL OTP (250uL of Cal5 + 250 uL DCM(14647)	G:\Org\HP5\Methods\DS_8015-JA-L#.met	1	1	1	1	0
	G:\org\HP5\DAT\HP5011122_b\0111HP5.08r	CCV_0111HP508r, CAL5 ;0111HP5 , 1000 ug per mL OTP (250 uL 4000 ug/mL OTP DRO211101A + 750 DCM(14647)	G:\Org\HP5\Methods\DS_8015-JA-L#.met	1	1	1	1	0
	G:\org\HP5\DAT\HP5011122_b\0111HP5.09r	CCV_0111HP509r, CAL1 ;0111HP5 , 150 ug per mL Diesel (20 uL of Cal3 + 980 uL DCM(14647), then 100 uL of that + 100 uL of DCM (14647)	G:\Org\HP5\Methods\DC_8015-JA-L%.met	1	1	1	1	0
	G:\org\HP5\DAT\HP5011122_b\0111HP5.10r	CCV_0111HP510r, CAL2 ;0111HP5 , 3750 ug per mL Diesel (100 uL Cal4 + 900 uL of DCM(14647)	G:\Org\HP5\Methods\DC_8015-JA-L%.met	1	1	1	1	0
	G:\org\HP5\DAT\HP5011122_b\0111HP5.11r	CCV_0111HP511r, CAL3 ;0111HP5 , 15000 ug per mL Diesel (300 uL of DRO211214C + 700 uL DCM(14647)	G:\Org\HP5\Methods\DC_8015-JA-L%.met	1	1	1	1	0
	G:\org\HP5\DAT\HP5011122_b\0111HP5.12r	CCV_0111HP512r, CAL4 ;0111HP5 , 37500ug per mL Diesel (750 uL of DRO211214C + 250 uL DCM(14647)	G:\Org\HP5\Methods\DC_8015-JA-L%.met	1	1	1	1	0
	G:\org\HP5\DAT\HP5011122_b\0111HP5.13r	CCV_0111HP513r, CAL5 ;0111HP5 , 50000 ug per mL Diesel (200 uL of DRO211214C)	G:\Org\HP5\Methods\DC_8015-JA-L%.met	1	1	1	1	0
	G:\org\HP5\DAT\HP5011122_b\0111HP5.14r	CCV_0111HP514r, Second Source ;0111HP5 , 15000 ug per mL (100uL of DRO211012B + 900uL DCM(14647)	G:\Org\HP5\Methods\DC_8015-JA-L%.met	1	1	1	1	0



File Name: G:\Org\HP5\Cals\SW8015C\_DRO220111JA.CAL

Version: 12

Creator: AMN 01/13/2022

Description: 8015C-DRO. New ICal Per 0111HP5 (2022)-2 uL Inj.; COD added using OTP RFs

Reason for change:

External standard calibration

Standard injection volume: 1

Standard sample weight: 1

Area reject threshold: 500

Reference peak area reject threshold: 500

Amount units: nanograms


No default component

Method of calculating data point averages: Equal weight for all updates

No calibration update report

All levels are normal data points.

1 DRO Range Start

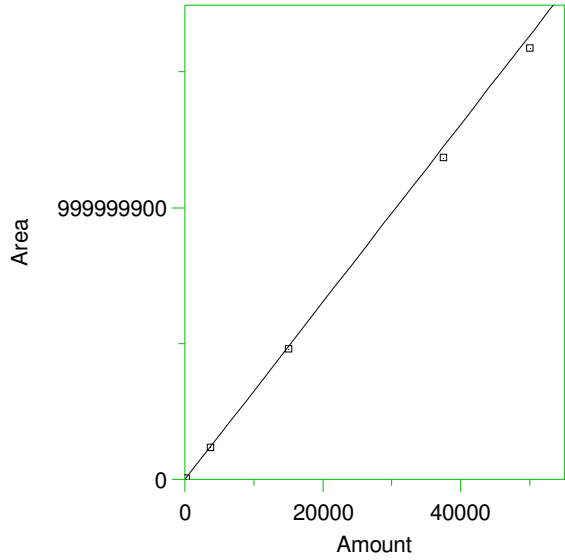

Expected retention time: 6.68 minutes  
 Search window: 0.05 minutes  
 No retention time reference component  
 Group number: 0  
 High alarm limit: 0  
 Low alarm limit: 0  
 Component constant: 0


Single peak quantification by area

$Y = 32675.36 X + 0$

Average CF fit with equal weighting, forced to origin  
 Coefficient of determination: 0.9980255  
 Average error: 3.607%  
 Average CF: 32675.36  
 RSD: 5.100%

Level	Amount	Response	Cal Factor	Error, %	Source	Date and time
1	150	5343235	35621.57	9.017	Manual	1/13/2022 12:28:36 PM
2	3750	1.20843E+08	32224.8	-1.379	Manual	1/13/2022 12:29:11 PM
3	15000	4.82244E+08	32149.6	-1.609	Manual	1/13/2022 12:29:24 PM
4	37500	1.185834E+09	31622.24	-3.223	Manual	1/13/2022 12:29:37 PM
5	50000	1.58793E+09	31758.6	-2.806	Manual	1/13/2022 12:28:57 PM


2 \*o-Terphenyl



Expected retention time: 12.35 minutes  
 Search window: 0.05 minutes  
 No retention time reference component  
 Group number: 0  
 High alarm limit: 0  
 Low alarm limit: 0  
 Component constant: 0  
 Single peak quantification by area  
 $Y = 36857.86 X + 0$   
 Average CF fit with equal weighting, forced to origin  
 Coefficient of determination: 0.9995278  
 Average error: 1.804%  
 Average CF: 36857.86  
 RSD: 2.132%

Level	Amount	Response	Cal Factor	Error, %	Source	Date and time
1	2	74333.97	37166.98	0.839	G:\Org\HP5\DAT\HP5011122_b\0111HP5.0004.BND	1/13/2022 12:27:15 PM
2	50	1802420	36048.4	-2.196	G:\Org\HP5\DAT\HP5011122_b\0111HP5.0005.BND	1/13/2022 12:27:23 PM
3	200	7546240	37731.2	2.369	G:\Org\HP5\DAT\HP5011122_b\0111HP5.0006.BND	1/13/2022 12:27:28 PM
4	500	1.800271E+07	36005.42	-2.313	G:\Org\HP5\DAT\HP5011122_b\0111HP5.0007.BND	1/13/2022 12:27:34 PM
5	1000	3.733731E+07	37337.31	1.301	G:\Org\HP5\DAT\HP5011122_b\0111HP5.0008.BND	1/13/2022 12:27:40 PM

3 \*1-Chlorooctadecane

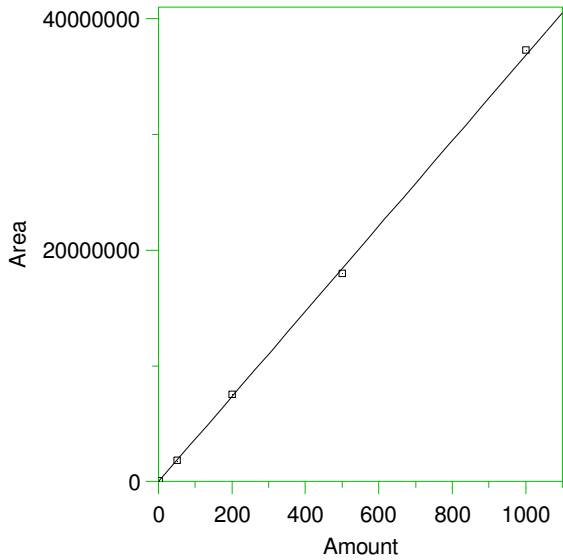

Expected retention time: 13.16 minutes  
 Search window: 0.05 minutes  
 No retention time reference component  
 Group number: 0  
 High alarm limit: 0  
 Low alarm limit: 0  
 Component constant: 0  
 Single peak quantification by area  
 Y = 36857.86 X + 0  
 Average CF fit with equal weighting, forced to origin  
 Coefficient of determination: 0.9995278  
 Average error: 1.804%  
 Average CF: 36857.86  
 RSD: 2.132%

Level	Amount	Response	Cal Factor	Error, %	Source	Date and time
1	2	74333.97	37166.98	0.839	Manual	1/13/2022 12:27:45 PM
2	50	1802420	36048.4	-2.196	Manual	1/13/2022 12:27:47 PM
3	200	7546240	37731.2	2.369	Manual	1/13/2022 12:27:49 PM
4	500	1.800271E+07	36005.42	-2.313	Manual	1/13/2022 12:27:51 PM
5	1000	3.733731E+07	37337.31	1.301	Manual	1/13/2022 12:27:53 PM

Write Sequence	Data File	Sample Name	Method	Weight	Dil Factor	Amt Inj.	IS	Cal ID	Manual Integrations
		DCM-Baseline Check-V01	G:\Org\HP5-Methods\DR_8015-IC-LEXP.met	1	1	1	1	0	No Integration
		CCV_0111HP502r, DRO ;0111HP5 , DRO220102D	G:\Org\HP5-Methods\DC_8015-JA-L%.met	1	1	1	1	0	No Integration
		DCM-Baseline Check-V03	G:\Org\HP5-Methods\DR_8015-IC-LEXP.met	1	1	1	1	0	No Integration
		CCV_0111HP504r, CAL1 ;0111HP5 , 2 ug per mL OTP (10 uL of Cal3 + 990 uL DCM(14647)	G:\Org\HP5-Methods\DS_8015-JA-L#.met	1	1	1	1	0	Surrogates are integrated using a valley to valley integration Set Baseline All Valley on at 12.01 minutes.
		CCV_0111HP505r, CAL2 ;0111HP5 , 50 ug per mL OTP (100 uL Cal4 + 900 uL of DCM(14647)	G:\Org\HP5-Methods\DS_8015-JA-L#.met	1	1	1	1	0	Surrogates are integrated using a valley to valley integration Set Baseline All Valley on at 12.01 minutes.
		CCV_0111HP506r, CAL3 ;0111HP5 , 200 ug per mL OTP (100uL of Cal5 + 400 uL DCM(14647)	G:\Org\HP5-Methods\DS_8015-JA-L#.met	1	1	1	1	0	Surrogates are integrated using a valley to valley integration Set Baseline All Valley on at 12.01 minutes.
		CCV_0111HP507r, CAL4 ;0111HP5 , 500 ug per mL OTP (250uL of Cal5 + 250 uL DCM(14647)	G:\Org\HP5-Methods\DS_8015-JA-L#.met	1	1	1	1	0	Surrogates are integrated using a valley to valley integration Set Baseline All Valley on at 12.01 minutes.
		CCV_0111HP508r, CAL5 ;0111HP5 , 1000 ug per mL OTP (250 uL 4000 ug/mL OTP DRO211101A + 750 DCM(14647)	G:\Org\HP5-Methods\DS_8015-JA-L#.met	1	1	1	1	0	Surrogates are integrated using a valley to valley integration Set Baseline All Valley on at 12.01 minutes.
		CCV_0111HP509r, CAL1 ;0111HP5 , 150 ug per mL Diesel (20 uL of Cal3 + 980 uL DCM(14647), then 100 uL of that + 100 uL of DCM (14647))	G:\Org\HP5-Methods\DC_8015-JA-L%.met	1	1	1	1	0	The integration of Diesel Range Organics and Total Extractable Hydrocarbons is the hydrocarbon response with reference to the baseline. Assigned Set Baseline on All Valley on at 16.36 minutes.
		CCV_0111HP510r, CAL2 ;0111HP5 , 3750 ug per mL Diesel (100 uL Cal4 + 900 uL of DCM(14647)	G:\Org\HP5-Methods\DC_8015-JA-L%.met	1	1	1	1	0	The integration of Diesel Range Organics and Total Extractable Hydrocarbons is the hydrocarbon response with reference to the baseline. Assigned Set Baseline on All Valley on at 16.36 minutes.
		CCV_0111HP511r, CAL3 ;0111HP5 , 15000 ug per mL Diesel (300 uL of DRO211214C + 700 uL DCM(14647)	G:\Org\HP5-Methods\DC_8015-JA-L%.met	1	1	1	1	0	The integration of Diesel Range Organics and Total Extractable Hydrocarbons is the hydrocarbon response with reference to the baseline. Assigned Set Baseline on All Valley on at 16.36 minutes.
		CCV_0111HP512r, CAL4 ;0111HP5 , 37500ug per mL Diesel (750 uL of DRO211214C + 250 uL DCM(14647)	G:\Org\HP5-Methods\DC_8015-JA-L%.met	1	1	1	1	0	The integration of Diesel Range Organics and Total Extractable Hydrocarbons is the hydrocarbon response with reference to the baseline. Assigned Set Baseline on All Valley on at 16.36 minutes.
		CCV_0111HP513r, CAL5 ;0111HP5 , 50000 ug per mL Diesel (200 uL of DRO211214C)	G:\Org\HP5-Methods\DC_8015-JA-L%.met	1	1	1	1	0	The integration of Diesel Range Organics and Total Extractable Hydrocarbons is the hydrocarbon response with reference to the baseline. Assigned Set Baseline on All Valley on at 16.36 minutes.
		CCV_0111HP514r, Second Source ;0111HP5 , 15000 ug per mL (100uL of DRO211012B + 900uL DCM(14647)	G:\Org\HP5-Methods\DC_8015-JA-L%.met	1	1	1	1	0	The integration of Diesel Range Organics and Total Extractable Hydrocarbons is the hydrocarbon response with reference to the baseline. Assigned Set Baseline on All Valley on at 16.36 minutes.

*Ann Nebel*

Digitally signed by  
Ann Nebel  
Date: 2022.02.11 10:29:19 -07:00

Write Sequence	Data File	Sample Name	Method	Weight	Dil Factor	Amt Inj.	IS	Cal ID	Manual Integrations
		DCM-Baseline Check-V01	G:\Org\HP5-Methods\DR_8015-IC-LEXP.met	1	1	1	1	0	No Integration
		CCV_0111HP502r, DRO_0111HP5, DRO220102D	G:\Org\HP5-Methods\DC_8015-JA-L%.met	1	1	1	1	0	No Integration
		DCM-Baseline Check-V03	G:\Org\HP5-Methods\DR_8015-IC-LEXP.met	1	1	1	1	0	No Integration
		CCV_0111HP504r, CAL1_0111HP5, 2 ug per mL OTP (10 uL of Cal3 + 990 uL DCM(14647))	G:\Org\HP5-Methods\DS_8015-JA-L#.met	1	1	1	1	0	Surrogates are integrated using a valley to valley integration Set Baseline All Valley on at 12.01 minutes.
		CCV_0111HP505r, CAL2_0111HP5, 50 ug per mL OTP (100 uL Cal4 + 900 uL DCM(14647))	G:\Org\HP5-Methods\DS_8015-JA-L#.met	1	1	1	1	0	Surrogates are integrated using a valley to valley integration Set Baseline All Valley on at 12.01 minutes.
		CCV_0111HP506r, CAL3_0111HP5, 200 ug per mL OTP (100uL of Cal5 + 400 uL DCM(14647))	G:\Org\HP5-Methods\DS_8015-JA-L#.met	1	1	1	1	0	Surrogates are integrated using a valley to valley integration Set Baseline All Valley on at 12.01 minutes.
		CCV_0111HP507r, CAL4_0111HP5, 500 ug per mL OTP (250uL of Cal5 + 250 uL DCM(14647))	G:\Org\HP5-Methods\DS_8015-JA-L#.met	1	1	1	1	0	Surrogates are integrated using a valley to valley integration Set Baseline All Valley on at 12.01 minutes.
		CCV_0111HP508r, CAL5_0111HP5, 1000 ug per mL OTP (250 uL 4000 ug/mL OTP DRO211101A + 750 DCM(14647))	G:\Org\HP5-Methods\DS_8015-JA-L#.met	1	1	1	1	0	Surrogates are integrated using a valley to valley integration Set Baseline All Valley on at 12.01 minutes.
		CCV_0111HP509r, CAL1_0111HP5, 150 ug per mL Diesel (20 uL of Cal3 + 980 uL DCM(14647)), then 100 uL of that + 100 uL of DCM (14647))	G:\Org\HP5-Methods\DC_8015-JA-L%.met	1	1	1	1	0	The integration of Diesel Range Organics and Total Extractable Hydrocarbons is the hydrocarbon response with reference to the baseline. Assigned Set Baseline on All Valley on at 16.36 minutes.
		CCV_0111HP510r, CAL2_0111HP5, 3750 ug per mL Diesel (100 uL Cal4 + 900 uL of DCM(14647))	G:\Org\HP5-Methods\DC_8015-JA-L%.met	1	1	1	1	0	The integration of Diesel Range Organics and Total Extractable Hydrocarbons is the hydrocarbon response with reference to the baseline. Assigned Set Baseline on All Valley on at 16.36 minutes.
		CCV_0111HP511r, CAL3_0111HP5, 15000 ug per mL Diesel (300 uL of DRO211214C + 700 uL DCM(14647))	G:\Org\HP5-Methods\DC_8015-JA-L%.met	1	1	1	1	0	The integration of Diesel Range Organics and Total Extractable Hydrocarbons is the hydrocarbon response with reference to the baseline. Assigned Set Baseline on All Valley on at 16.36 minutes.
		CCV_0111HP512r, CAL4_0111HP5, 37500ug per mL Diesel (750 uL of DRO211214C + 250 uL DCM(14647))	G:\Org\HP5-Methods\DC_8015-JA-L%.met	1	1	1	1	0	The integration of Diesel Range Organics and Total Extractable Hydrocarbons is the hydrocarbon response with reference to the baseline. Assigned Set Baseline on All Valley on at 16.36 minutes.
		CCV_0111HP513r, CAL5_0111HP5, 50000 ug per mL Diesel (200 uL of DRO211214C)	G:\Org\HP5-Methods\DC_8015-JA-L%.met	1	1	1	1	0	The integration of Diesel Range Organics and Total Extractable Hydrocarbons is the hydrocarbon response with reference to the baseline. Assigned Set Baseline on All Valley on at 16.36 minutes.
		CCV_0111HP514r, Second Source_0111HP5, 15000 ug per mL (100uL of DRO211012B + 900uL DCM(14647))	G:\Org\HP5-Methods\DC_8015-JA-L%.met	1	1	1	1	0	The integration of Diesel Range Organics and Total Extractable Hydrocarbons is the hydrocarbon response with reference to the baseline. Assigned Set Baseline on All Valley on at 16.36 minutes.

*Ann Nebel*

Digitally signed by  
Ann Nebel  
Date: 2022.02.11 10:29:19 -07:00

# Energy Laboratories Inc

# ANALYTICAL RUN Summary

14-Jan-22

Run ID GCFID-HP5-B\_220111C

<b>Run Start Date:</b> 1/11/2022
<b>Analyst:</b> Ann Nebel
<b>Ical:</b>
<b>Column ID:</b>
<b>Comments:</b> ICAL- SW8015C_ORO220111BA.CAL with Triacontane

Std ID	Std Name	Std Amount	Std Units	Samp Amount	Samp Units	SampType	Expiration Date
DRO210902A	50,000 ug/mL Oil Std for RRO-In DCM					ICV	9/1/2026
DRO211006A	Triacontane SURR 2000 ug/mL					CAL-SURR	4/6/2026
DRO211118A	50,000 ug/mL Oil Std For AK103 RRO-In DCM					CAL-ORO	10/31/2028

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977288	CCV_0111HP52	HC-8015-DRO-	CAL1		1/12/2022 3:39:1	1	R373160		0	0						
<b>Analyte</b>	<b>T</b>	<b>Units</b>	<b>RAW</b>	<b>Final</b>	<b>Text</b>	<b>Spike</b>	<b>SPKref</b>	<b>RPDref</b>	<b>MDL</b>	<b>PQL</b>	<b>UQL</b>	<b>%REC</b>	<b>LOW</b>	<b>HIGH</b>	<b>%RPD</b>	<b>Q</b>
n-Triacontane	S	mg/L	0.00190245			0.002	0	0	0.000336	0.002	0	95%	80	120	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977289	CCV_0111HP52	HC-8015-DRO-	CAL2		1/12/2022 4:22:1	1	R373160		0	0						
<b>Analyte</b>	<b>T</b>	<b>Units</b>	<b>RAW</b>	<b>Final</b>	<b>Text</b>	<b>Spike</b>	<b>SPKref</b>	<b>RPDref</b>	<b>MDL</b>	<b>PQL</b>	<b>UQL</b>	<b>%REC</b>	<b>LOW</b>	<b>HIGH</b>	<b>%RPD</b>	<b>Q</b>
n-Triacontane	S	mg/L	0.04984459			0.05	0	0	0.000336	0.002	0	100%	80	120	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977290	CCV_0111HP53	HC-8015-DRO-	CAL3		1/12/2022 5:05:2	1	R373160		0	0						
<b>Analyte</b>	<b>T</b>	<b>Units</b>	<b>RAW</b>	<b>Final</b>	<b>Text</b>	<b>Spike</b>	<b>SPKref</b>	<b>RPDref</b>	<b>MDL</b>	<b>PQL</b>	<b>UQL</b>	<b>%REC</b>	<b>LOW</b>	<b>HIGH</b>	<b>%RPD</b>	<b>Q</b>
n-Triacontane	S	mg/L	0.2024053			0.2	0	0	0.000336	0.002	0	101%	80	120	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977291	CCV_0111HP53	HC-8015-DRO-	CAL4		1/12/2022 5:48:3	1	R373160		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
n-Triacontane	S	mg/L		0.5035697		0.5	0	0	0.000336	0.002	0	101%	80	120	0%	
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977292	CCV_0111HP55	HC-8015-DRO-	CAL5		1/12/2022 8:49:5	1	R373160		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
n-Triacontane	S	mg/L		1.032718		1	0	0	0.000336	0.002	0	103%	80	120	0%	
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977293	CCV_0111HP55	HC-8015-DRO-	CAL1		1/13/2022 3:06:1	1	R373160		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
TEH(Oil Range)	A	mg/L		0.15954587		0.15	0	0	0.0879	0.3	0	106%	80	120	0%	
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977294	CCV_0111HP55	HC-8015-DRO-	CAL2		1/13/2022 4:31:3	1	R373160		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
TEH(Oil Range)	A	mg/L		1.03294141		1	0	0	0.0879	0.3	0	103%	80	120	0%	
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977295	CCV_0111HP55	HC-8015-DRO-	CAL3		1/13/2022 5:57:4	1	R373160		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
TEH(Oil Range)	A	mg/L		4.9326875		5	0	0	0.0879	0.3	0	99%	80	120	0%	
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977296	CCV_0111HP56	HC-8015-DRO-	CAL4		1/13/2022 7:24:1	1	R373160		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
TEH(Oil Range)	A	mg/L		14.328667		15	0	0	0.0879	0.3	0	96%	80	120	0%	



Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977297	CCV_0111HP56	HC-8015-DRO-	CAL5		1/13/2022 8:50:3	1	R373160		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
TEH(Oil Range)	A	mg/L		28.7914395		30	0	0	0.0879	0.3	0	96%	80	120	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14977298	CCV_0111HP56	HC-8015-DRO-	ICV		1/14/2022 8:18:1	0	R373160		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
TEH(Oil Range)	A	mg/L		5.07699902		5	0	0	0	0.3	0	102%	80	120	0%	

Write Sequence	Data File	Sample Name	Method	Weight	Dil Factor	Amt Inj.	IS	Cal ID
	b\0111HP5.25f	DCM-Baseline Check-V25	G:\Org\HP5\Methods\DR_8015-IC-LEXP.met	1	1	1	1	0
	b\0111HP5.26f	Marker_0111HP526r, DRO :0111HP5 , DRO220111A	G:\Org\HP5\Methods\CSC210212.met	1	1	1	1	0
	b\0111HP5.27f	DCM-Baseline Check-V27	G:\Org\HP5\Methods\DR_8015-HS-LEXP.met	1	1	1	1	0
	b\0111HP5.28f	CCV_0111HP528r, CAL1 :0111HP5 , 2 ug per mL Triacotane (10 uL of Cal3 + 990 uL DCM(14647)	G:\Org\HP5\Methods\DS_ORO-BA-L#.MET	1	1	1	1	0
	b\0111HP5.29f	CCV_0111HP529r, CAL2 :0111HP5 , 50 ug per mL Triacotane (100 uL Cal4 + 900 uL of DCM(14647)	G:\Org\HP5\Methods\DS_ORO-BA-L#.MET	1	1	1	1	0
	b\0111HP5.30f	CCV_0111HP530r, CAL3 :0111HP5 , 200 ug per mL Triacotane (100uL of Cal5 + 400 uL DCM(14647)	G:\Org\HP5\Methods\DS_ORO-BA-L#.MET	1	1	1	1	0
	b\0111HP5.31f	CCV_0111HP531r, CAL4 :0111HP5 , 500 ug per mL Triacotane (250uL of Cal5 + 250 uL DCM(14647)	G:\Org\HP5\Methods\DS_ORO-BA-L#.MET	1	1	1	1	0
	b\0111HP5.32f	DCM-Baseline Check-V32	G:\Org\HP5\Methods\DR_8015-HE-LEXP.met	1	1	1	1	0
	b\0111HP5.50f	CCV_0111HP550r, CAL5 :0111HP5 , 1000 ug per mL Triacotane (DRO211006A)	G:\Org\HP5\Methods\DS_ORO-BA-L#.MET	1	1	1	1	0
	b\0111HP5.51f	DCM-Baseline Check-V51	G:\Org\HP5\Methods\DR_8015-IC-LEXP.met	1	1	1	1	0
	b\0111HP5.52f	DCM-Baseline Check-V52	G:\Org\HP5\Methods\DR_8015-IC-LEXP.met	1	1	1	1	0
	b\0111HP5.53f	Marker_0111HP553r, DRO :0111HP5 , DRO220111A	G:\Org\HP5\Methods\CSC210212.met	1	1	1	1	0
	b\0111HP5.54f	DCM-Baseline Check-V54	G:\Org\HP5\Methods\DR_8015-IC-LEXP.met	1	1	1	1	0
	b\0111HP5.55f	CCV_0111HP555r, CAL1 :0111HP5 , 150 ug per mL Oil (10 uL of Cal4 + 990 uL DCM(14647)	G:\Org\HP5\Methods\DC_ORO-55-BA-L%.xls	1	1	1	1	0
	b\0111HP5.56f	DCM-Baseline Check-V56	G:\Org\HP5\Methods\DR_8015-HE-LEXP.met	1	1	1	1	0
	b\0111HP5.57f	CCV_0111HP557r, CAL2 :0111HP5 , 1000 ug per mL Oil (200 uL of Cal 3 +800 uL DCM(14647)	G:\Org\HP5\Methods\DC_ORO-57-BA-L%.xls	1	1	1	1	0
	b\0111HP5.58f	DCM-Baseline Check-V58	G:\Org\HP5\Methods\DR_8015-HE-LEXP.met	1	1	1	1	0
	b\0111HP5.59f	CCV_0111HP559r, CAL3 :0111HP5 , 5000 ug per mL Oil (100 uL of DRO211118A + 900 uL DCM(14647)	G:\Org\HP5\Methods\DC_ORO-59-BA-L%.xls	1	1	1	1	0
	b\0111HP5.60f	DCM-Baseline Check-V60	G:\Org\HP5\Methods\DR_8015-HE-LEXP.met	1	1	1	1	0
	b\0111HP5.61f	CCV_0111HP561r, CAL4 :0111HP5 , 15000 ug per mL Oil (200 uL of CAL5 + 200 uL DCM(14647)	G:\Org\HP5\Methods\DC_ORO-61-BA-L%.xls	1	1	1	1	0
	b\0111HP5.62f	DCM-Baseline Check-V62	G:\Org\HP5\Methods\DR_8015-HE-LEXP.met	1	1	1	1	0
	b\0111HP5.63f	CCV_0111HP563r, CAL5 :0111HP5 , 30000 ug per mL Oil (600 uL of DRO211118A + 400 uL of DCM)	G:\Org\HP5\Methods\DC_ORO-BA-L%.xls	1	1	1	1	0
	b\0111HP5.64f	DCM-Baseline Check-V64	G:\Org\HP5\Methods\DR_8015-HE-LEXP.met	1	1	1	1	0
	b\0111HP5.65f	DCM-Baseline Check-V65	G:\Org\HP5\Methods\DR_8015-HE-LEXP.met	1	1	1	1	0
	b\0111HP5.66f	DCM-Baseline Check-V66	G:\Org\HP5\Methods\DR_8015-HE-LEXP.met	1	1	1	1	0
	b\0111HP5.68f	DCM-Baseline Check-V68	G:\Org\HP5\Methods\DR_8015-IC-LEXP.met	1	1	1	1	0
	b\0111HP5.69f	CCV_0111HP567r, Second Source :0111HP5 , 5000 ug per mL (100uL of DRO210902A + 900uL DCM(14647)	G:\Org\HP5\Methods\DC_ORO-59-BA-L%.xls	1	1	1	1	0

File Name: G:\Org\HP5\Cals\SW8015C\_ORO220111BA.CAL  
Version: 11  
  
Creator: AMN  
Description: 8015C-Oil Range with Triacontane. New ICal Per 0111HP5,(2022)-2 uL Inj.;  
Reason for change:


External standard calibration

Standard injection volume: 1  
Standard sample weight: 1  
Area reject threshold: 500  
Reference peak area reject threshold: 500  
Amount units: nanograms  
No default component

Method of calculating data point averages: Equal weight for all updates  
No calibration update report

All levels are normal data points.

1 \*30-40 Motor Oil



Expected retention time: 6.4 minutes  
 Search window: 0.05 minutes  
 No retention time reference component  
 Group number: 0  
 High alarm limit: 0  
 Low alarm limit: 0  
 Component constant: 0


Single peak quantification by area

$Y = 26424.55 X + 0$

Average CF fit with equal weighting, forced to origin  
 Coefficient of determination: 0.9969108  
 Average error: 3.495%  
 Average CF: 26424.55  
 RSD: 4.293%

Level	Amount	Response	Cal Factor	Error, %	Source	Date and time
1	150	4177025	27846.83	5.382	Manual	1/14/2022 7:51:42 AM
2	1000	2.73111E+07	27311.1	3.355	Manual	1/14/2022 8:05:40 AM
3	5000	1.313247E+08	26264.94	-0.604	Manual	1/14/2022 8:05:24 AM
4	15000	3.796282E+08	25308.55	-4.223	Manual	1/14/2022 8:05:07 AM
5	30000	7.617404E+08	25391.35	-3.910	Manual	1/14/2022 8:04:35 AM


2 #C20

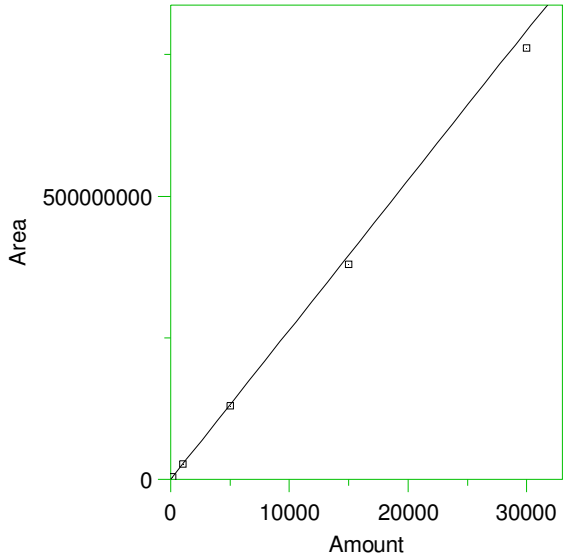

Expected retention time: 12.56 minutes  
 Search window: 0.05 minutes  
 No retention time reference component  
 Group number: 0  
 High alarm limit: 0  
 Low alarm limit: 0  
 Component constant: 0  
 Single peak quantification by area  
 $Y = 26424.55 X + 0$   
 Average CF fit with equal weighting, forced to origin  
 Coefficient of determination: 0.9969108  
 Average error: 3.495%  
 Average CF: 26424.55  
 RSD: 4.293%


Level	Amount	Response	Cal Factor	Error, %	Source	Date and time
1	150	4177025	27846.83	5.382	Manual	1/14/2022 8:06:03 AM
2	1000	2.73111E+07	27311.1	3.355	Manual	1/14/2022 8:06:05 AM
3	5000	1.313247E+08	26264.94	-0.604	Manual	1/14/2022 8:06:06 AM
4	15000	3.796282E+08	25308.55	-4.223	Manual	1/14/2022 8:06:11 AM
5	30000	7.617404E+08	25391.35	-3.910	Manual	1/14/2022 8:06:13 AM

3 \*#Triacontane



Expected retention time: 16.44 minutes  
 Search window: 0.05 minutes  
 No retention time reference component  
 Group number: 0  
 High alarm limit: 0  
 Low alarm limit: 0  
 Component constant: 0  
 Single peak quantification by area  
 Y = 29636.1 X + 0  
 Average CF fit with equal weighting, forced to origin  
 Coefficient of determination: 0.9984925  
 Average error: 2.075%  
 Average CF: 29636.1  
 RSD: 3.023%

Level	Amount	Response	Cal Factor	Error, %	Source	Date and time
1	2	56381.2	28190.6	-4.878	Manual	1/13/2022 12:38:47 PM
2	50	1477199	29543.98	-0.311	Manual	1/13/2022 12:38:50 PM
3	200	5998503	29992.52	1.203	Manual	1/13/2022 12:38:53 PM
4	500	1.492384E+07	29847.68	0.714	Manual	1/13/2022 12:38:56 PM
5	1000	3.060573E+07	30605.73	3.272	Manual	1/13/2022 12:39:03 PM

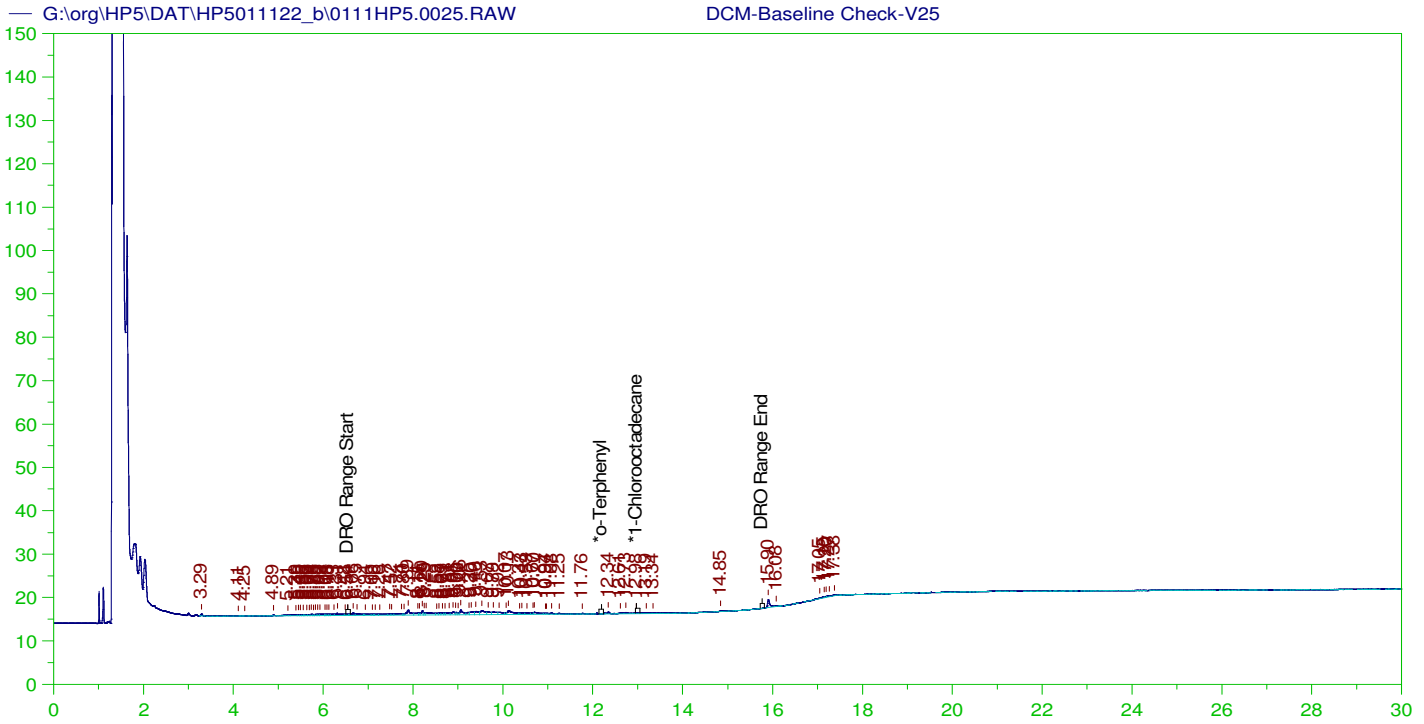


**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: DCM-Baseline Check-V25  
 Raw File: G:\Org\HP5\DAT\HP5011122\_b\0111HP5.0025.RAW  
 Date & Time Acquired: 1/12/2022 1:29:46 AM  
 Method File: G:\Org\HP5\Methods\DR\_8015-IC-LEXP.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO211102IC.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1


Mean RF for TEH: 31353.19  
 Rt range for Diesel Range Organics: 6.5 to 15.82

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	29.899	200.	.	-
*1-Chlorooctadecane	12.975	200.	.017	.01 -

DRO Area:132028.6 DRO Amount: 4.211011  
 TEH Area:186308.4 TEH Amount: 5.942247

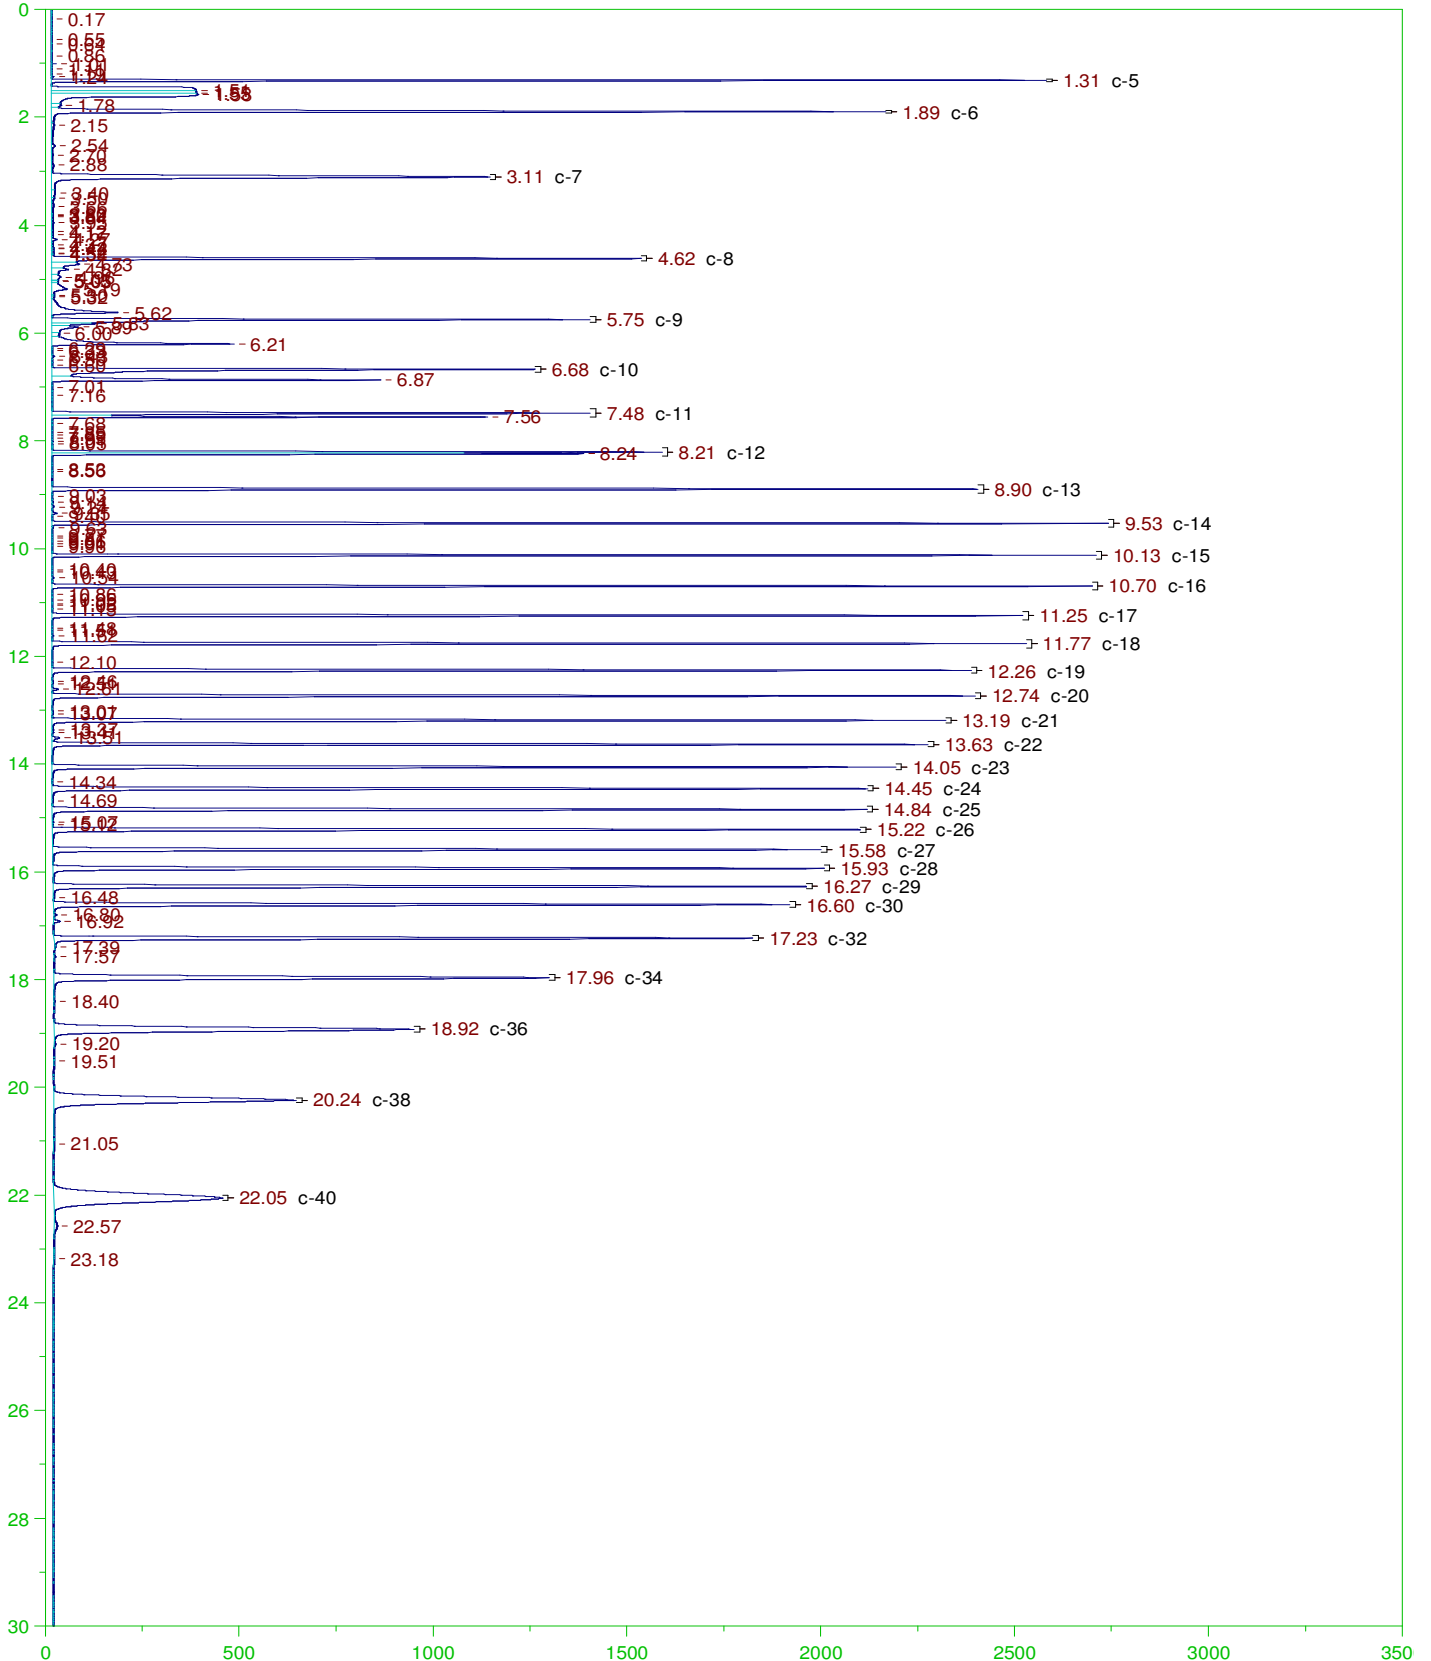





**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: DCM-Baseline Check-V27  
 Raw File: G:\org\HP5\DAT\HP5011122\_b\0111HP5.0027.RAW  
 Date & Time Acquired: 1/12/2022 2:56:04 AM  
 Method File: G:\Org\HP5\Methods\DR\_8015-HS-LEXP.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO210108Hs.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1


Mean RF for TEH: 29457.33  
 Rt range for Diesel Range Organics: 6.51 to 15.85

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.261	200.	.017	.01	-
*1-Chlorooctadecane	29.983	200.	.	.	-

DRO Area:193795.7 DRO Amount: 6.578862  
 TEH Area:272770 TEH Amount: 9.259835

G:\org\HP5\DAT\HP5011122\_b\0111HP5.0028.RAW

CCV\_0111HP528r, CAL1 ;0111HP5 , 2 ug per mL Triacontane

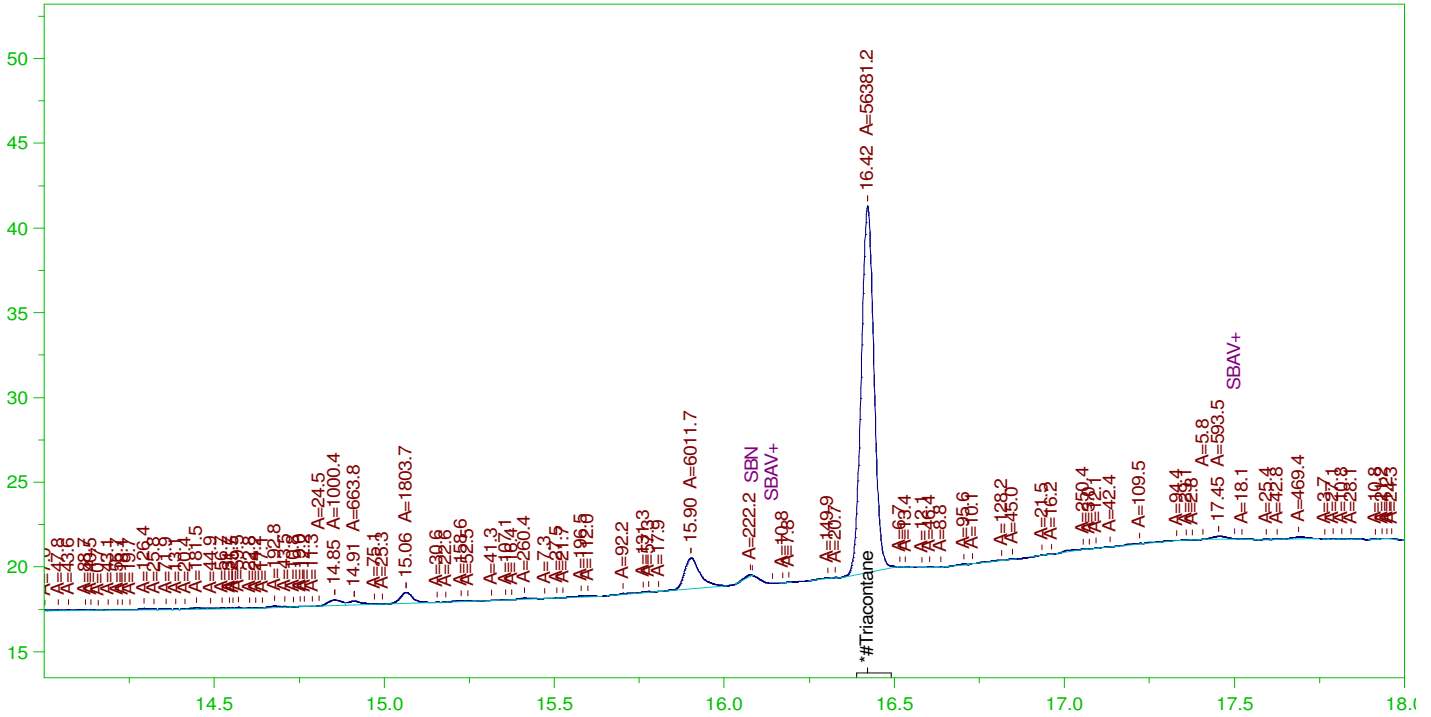

**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: CCV\_0111HP528r, CAL1 ;0111HP5 , 2 ug per mL Triacontane  
Raw File: G:\org\HP5\DAT\HP5011122\_b\0111HP5.0028.RAW  
Date & Time Acquired: 1/12/2022 3:39:11 AM  
Method File: G:\Org\HP5\Methods\DS\_ORO-BA-L%.MET  
Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111ba.CAL  
Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 28542.41  
Rt range for Residual Range Organics: 12.51 to 30.05

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*#Triacontane	16.421	500.	1.902	.38

RRO Area:11465.21 RRO AMOUNT: 0.4016902


CONTINUING CALIBRATION REPORT: G:\org\HP5\DAT\HP5011122\_b\0111HP5.0028.RAW

COMPOUND	ACTUAL (NG)	MEASURED (NG)	%RECOVERY	LIMITS
*30-40 Motor Oil	5000.	.056	.	75-125

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	LIMITS
*#Triacontane	16.421	200.	1.902	.95	75-125

G:\org\HP5\DAT\HP5011122\_b\0111HP5.0029.RAW

CCV\_0111HP529r, CAL2 ;0111HP5 , 50 ug per mL Triacontane

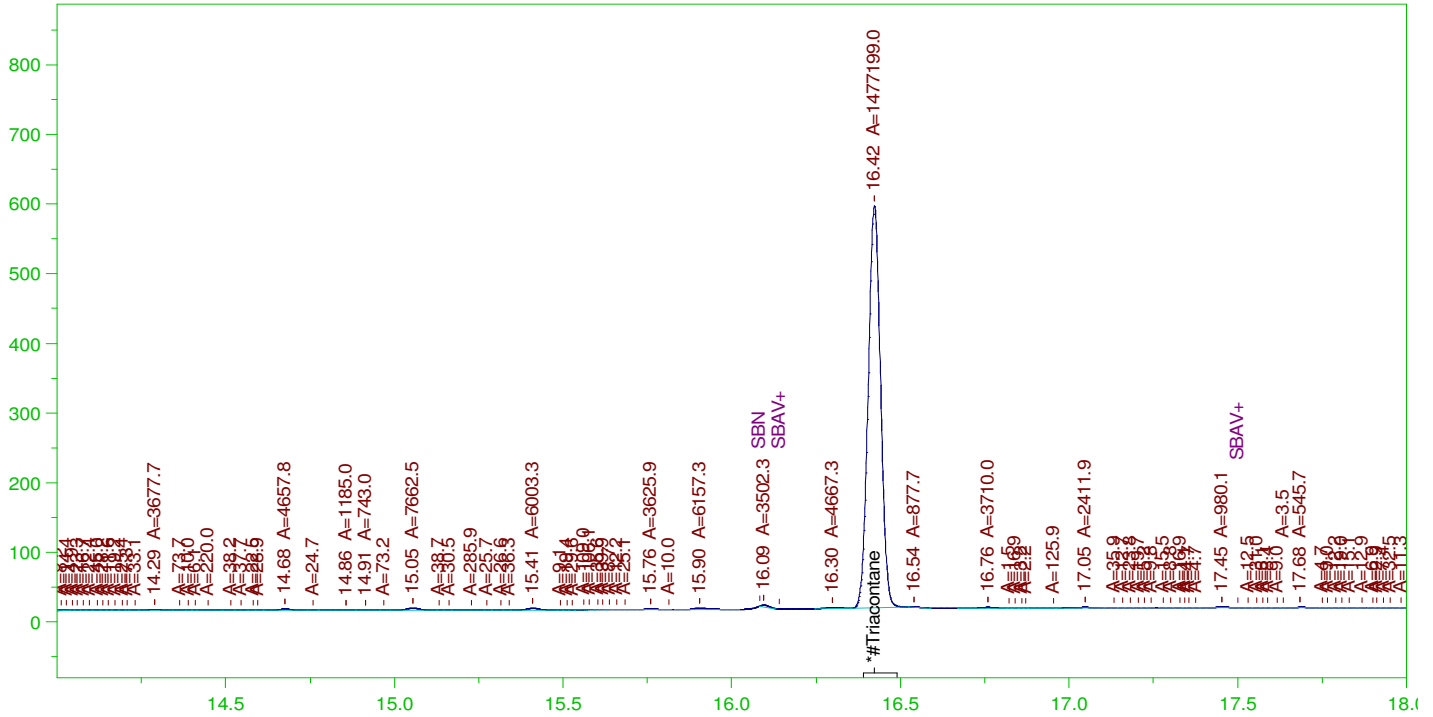

**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: CCV\_0111HP529r, CAL2 ;0111HP5 , 50 ug per mL Triacontane  
 Raw File: G:\org\HP5\DAT\HP5011122\_b\0111HP5.0029.RAW  
 Date & Time Acquired: 1/12/2022 4:22:15 AM  
 Method File: G:\Org\HP5\Methods\DS\_ORO-BA-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111ba.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 28542.41  
 Rt range for Residual Range Organics: 12.51 to 30.05

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*#Triacontane	16.423	500.	49.845	9.97


RRO Area:60154.51 RRO AMOUNT: 2.107548

CONTINUING CALIBRATION REPORT: G:\org\HP5\DAT\HP5011122\_b\0111HP5.0029.RAW

COMPOUND	ACTUAL (NG)	MEASURED (NG)	%RECOVERY	LIMITS
*30-40 Motor Oil	5000.	.023	.	75-125

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	LIMITS
*#Triacontane	16.423	200.	49.845	24.92	75-125

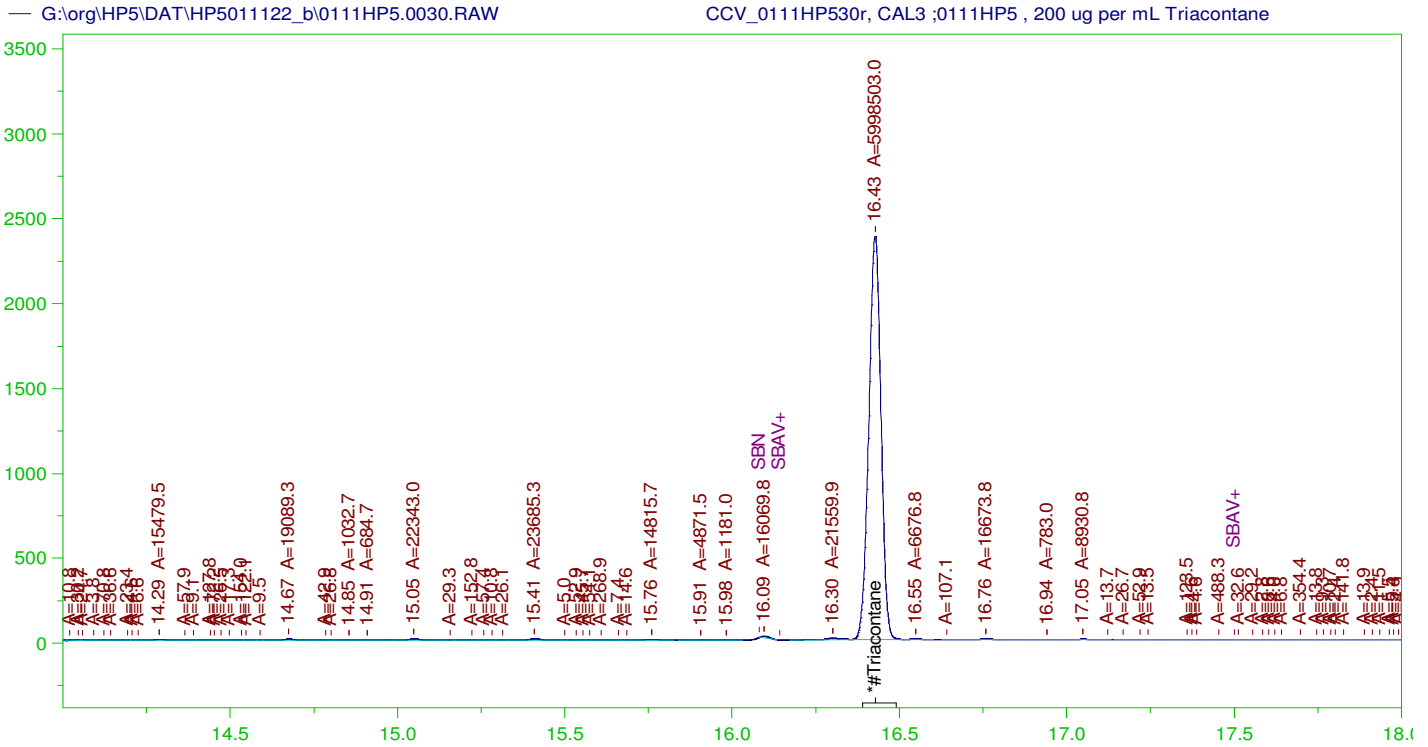

**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: CCV\_0111HP530r, CAL3 ;0111HP5 , 200 ug per mL Triacontane  
 Raw File: G:\org\HP5\DAT\HP5011122\_b\0111HP5.0030.RAW  
 Date & Time Acquired: 1/12/2022 5:05:25 AM  
 Method File: G:\Org\HP5\Methods\DS\_ORO-BA-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111ba.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 28542.41  
 Rt range for Residual Range Organics: 12.51 to 30.05

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*#Triacontane	16.427	500.	202.405	40.48	-

RRO Area:200104.8 RRO AMOUNT: 7.01079

CONTINUING CALIBRATION REPORT: G:\org\HP5\DAT\HP5011122\_b\0111HP5.0030.RAW


COMPOUND	ACTUAL (NG)	MEASURED (NG)	%RECOVERY	LIMITS
*30-40 Motor Oil	5000.	.	75-125	

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	LIMITS
*#Triacontane	16.427	200.	202.405	101.2	75-125

G:\org\HP5\DAT\HP5011122\_b\0111HP5.0031.RAW

CCV\_0111HP531r, CAL4 ;0111HP5 , 500 ug per mL Triacontane

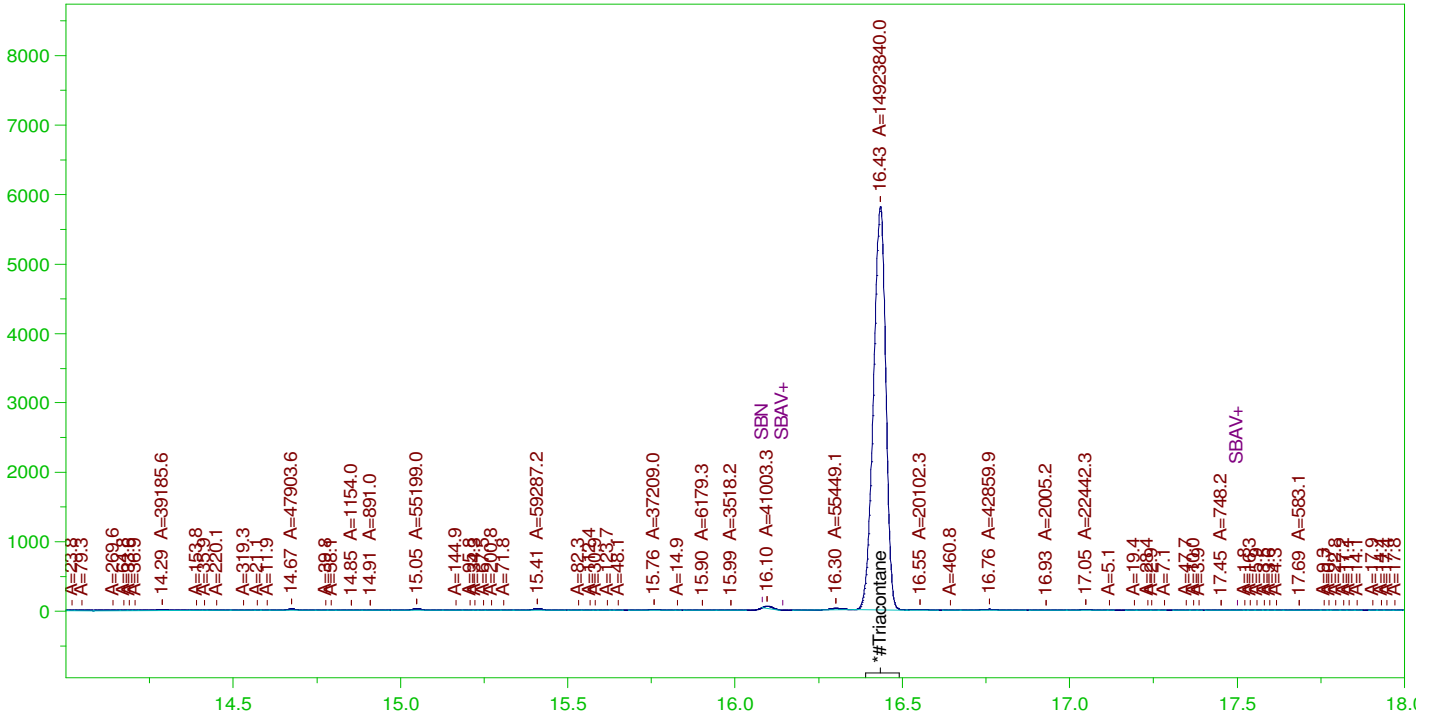

**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: CCV\_0111HP531r, CAL4 ;0111HP5 , 500 ug per mL Triacontane  
 Raw File: G:\org\HP5\DAT\HP5011122\_b\0111HP5.0031.RAW  
 Date & Time Acquired: 1/12/2022 5:48:34 AM  
 Method File: G:\Org\HP5\Methods\DS\_ORO-BA-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111ba.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 28542.41  
 Rt range for Residual Range Organics: 12.51 to 30.05

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*#Triacontane	16.434	500.	503.57	100.71	-


RRO Area:497882.9 RRO AMOUNT: 17.44362

CONTINUING CALIBRATION REPORT: G:\org\HP5\DAT\HP5011122\_b\0111HP5.0031.RAW  
 COMPOUND ACTUAL (NG) MEASURED (NG) %RECOVERY LIMITS  
 \*30-40 Motor Oil 5000. . . 75-125

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	LIMITS
*#Triacontane	16.434	200.	503.57	251.78	75-125

G:\org\HP5\DAT\HP5011122\_b\0111HP5.0050.RAW

CCV\_0111HP550r, CAL5 ;0111HP5 , 1000 ug per mL Triacontane



**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: CCV\_0111HP550r, CAL5 ;0111HP5 , 1000 ug per mL Triacontane  
 Raw File: G:\org\HP5\DAT\HP5011122\_b\0111HP5.0050.RAW  
 Date & Time Acquired: 1/12/2022 8:49:58 PM  
 Method File: G:\Org\HP5\Methods\DS\_ORO-BA-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111ba.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 28542.41  
 Rt range for Residual Range Organics: 12.51 to 30.05


SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*#Triacontane	16.444	500.	1032.718	206.54	-

RRO Area:993904.8 RRO AMOUNT: 34.82203

CONTINUING CALIBRATION REPORT: G:\org\HP5\DAT\HP5011122\_b\0111HP5.0050.RAW

COMPOUND	ACTUAL (NG)	MEASURED (NG)	%RECOVERY	LIMITS
*30-40 Motor Oil	5000.	.	75-125	

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	LIMITS
*#Triacontane	16.444	200.	1032.718	516.36	75-125

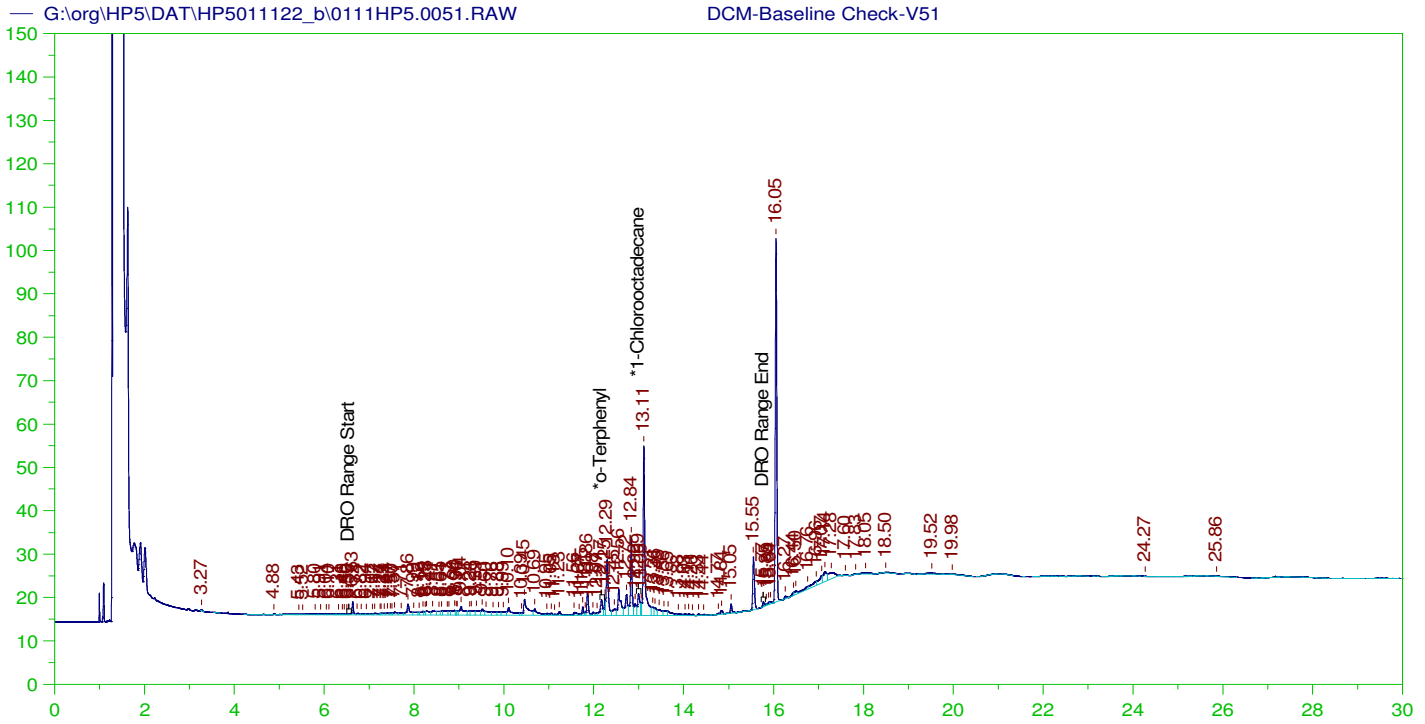


**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: DCM-Baseline Check-V51  
 Raw File: G:\org\HP5\DAT\HP5011122\_b\0111HP5.0051.RAW  
 Date & Time Acquired: 1/13/2022 12:15:29 PM  
 Method File: G:\Org\HP5\Methods\DR\_8015-IC-LEXP.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO211102IC.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for TEH: 31353.19  
 Rt range for Diesel Range Organics: 6.5 to 15.82

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.166	200.	.369	.18	-
*1-Chlorooctadecane	12.994	200.	.464	.23	-

DRO Area: 587062.5 DRO Amount: 18.72417  
 TEH Area: 891448.4 TEH Amount: 28.43246

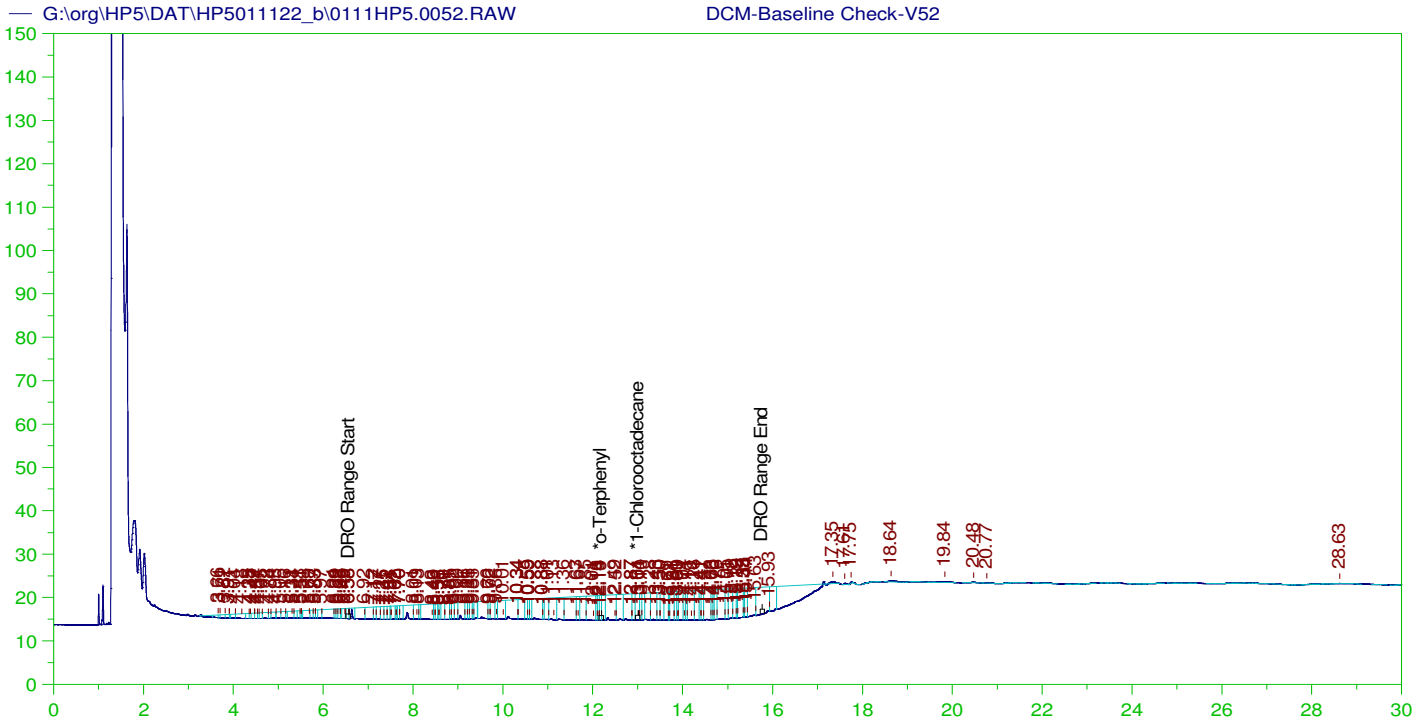

**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**


Sample Name: DCM-Baseline Check-V52  
 Raw File: G:\org\HP5\DAT\HP5011122\_b\0111HP5.0052.RAW  
 Date & Time Acquired: 1/13/2022 12:58:31 PM  
 Method File: G:\Org\HP5\Methods\DR\_8015-IC-LEXP.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO211102IC.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1


Mean RF for TEH: 31353.19  
 Rt range for Diesel Range Organics: 6.5 to 15.82

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.192	200.	.855	.43	-
*1-Chlorooctadecane	13.007	200.	.955	.48	-

DRO Area:2710300 DRO Amount: 86.44414  
 TEH Area:2842315 TEH Amount: 90.65472



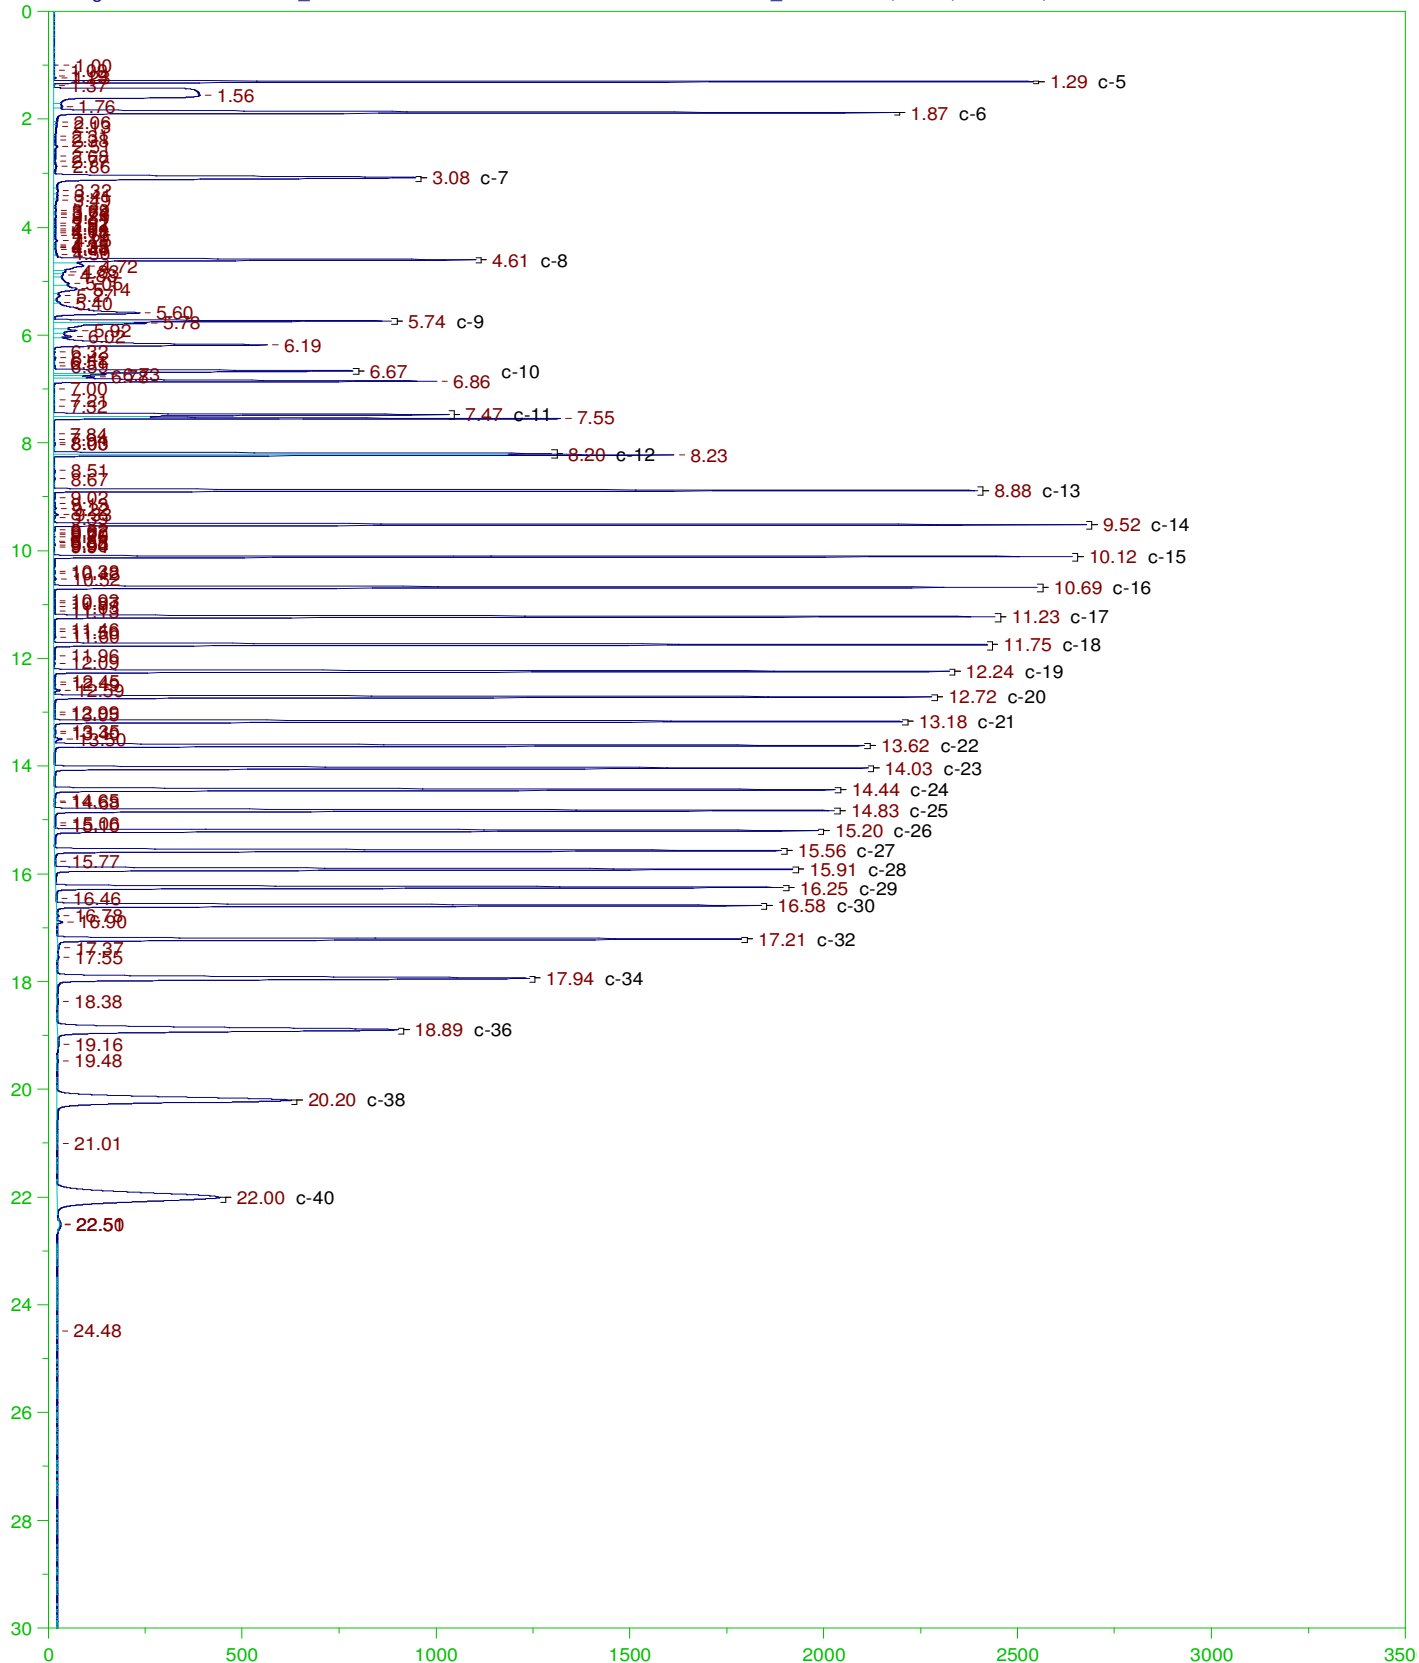

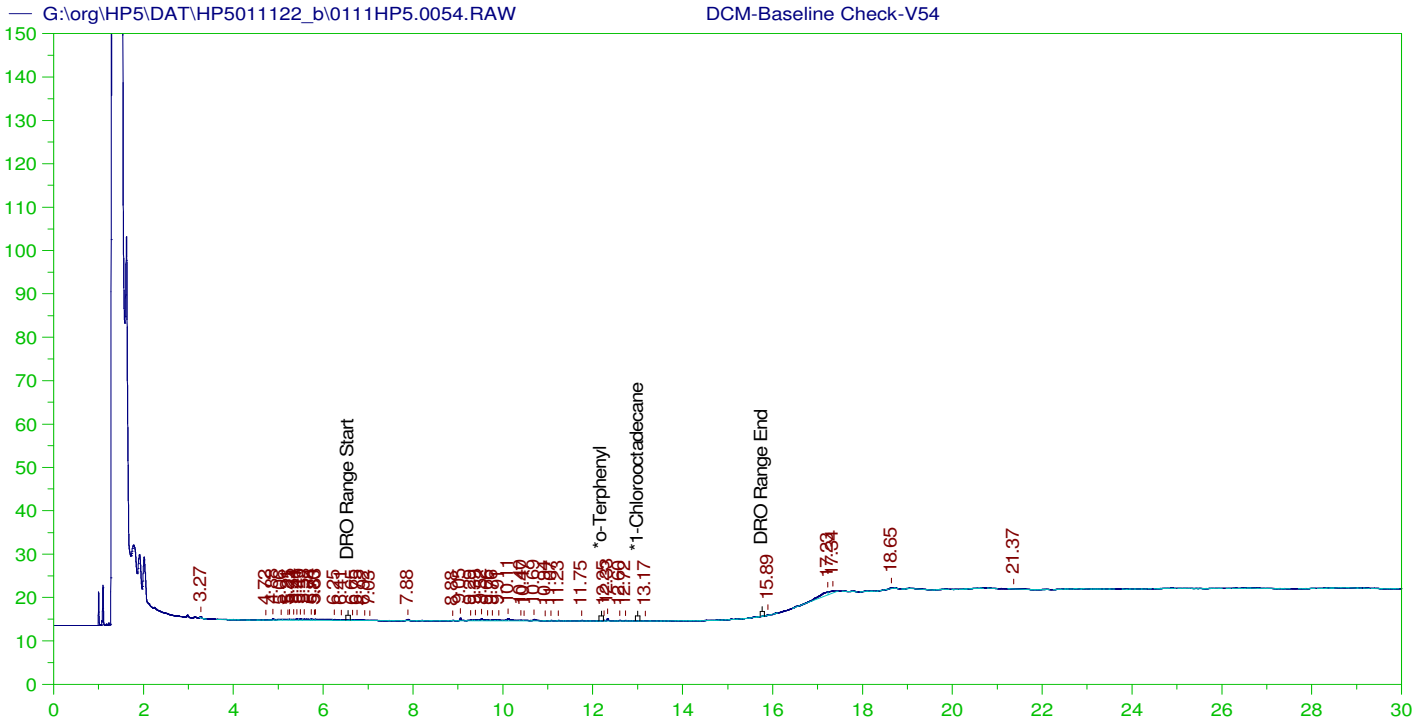


**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: DCM-Baseline Check-V54  
 Raw File: G:\org\HP5\DAT\HP5011122\_b\0111HP5.0054.RAW  
 Date & Time Acquired: 1/13/2022 2:23:42 PM  
 Method File: G:\Org\HP5\Methods\DR\_8015-IC-LEXP.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO211102IC.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for TEH: 31353.19  
 Rt range for Diesel Range Organics: 6.5 to 15.82

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	29.882	200.	.	-
*1-Chlorooctadecane	29.882	200.	.	-

DRO Area:44798.44 DRO Amount: 1.428832  
 TEH Area:97771.24 TEH Amount: 3.118382

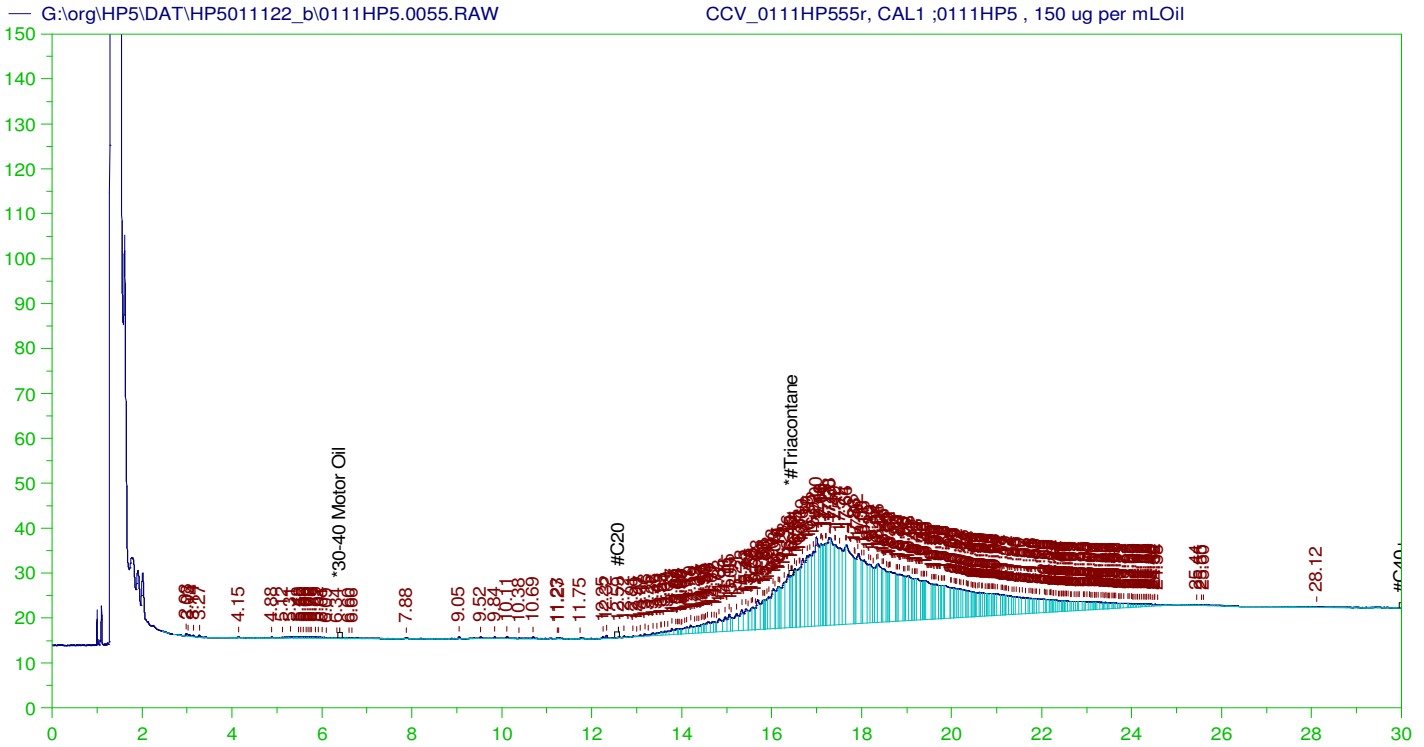

**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: CCV\_0111HP555r, CAL1 ;0111HP5 , 150 ug per mL Oil  
 Raw File: G:\org\HP5\DAT\HP5011122\_b\0111HP5.0055.RAW  
 Date & Time Acquired: 1/13/2022 3:06:11 PM  
 Method File: G:\Org\HP5\Methods\DC\_ORO-55-BA-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BA.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 26424.55  
 Rt range for Residual Range Organics: 12.51 to 30.05

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*#Triacontane	16.447	500.	.47	.09	-


RRO Area: 4215928 RRO AMOUNT: 159.5459

CONTINUING CALIBRATION REPORT: G:\org\HP5\DAT\HP5011122\_b\0111HP5.0055.RAW

COMPOUND	ACTUAL (NG)	MEASURED (NG)	%RECOVERY	LIMITS
*30-40 Motor Oil	5000.	.	75-125	

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	LIMITS
*#Triacontane	16.447	200.	.47	.23	75-125



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**


Sample Name: DCM-Baseline Check-V56  
 Raw File: G:\org\HP5\DAT\HP5011122\_b\0111HP5.0056.RAW  
 Date & Time Acquired: 1/13/2022 3:48:53 PM  
 Method File: G:\Org\HP5\Methods\DR\_8015-HE-LEXP.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO210108HE.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for TEH: 29457.33

Rt range for Diesel Range Organics: 6.49 to 15.75

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	12.162	200.	.406	.2
*1-Chlorooctadecane	29.946	200.	.	.

DRO Area:2125703 DRO Amount: 72.16209  
 TEH Area:2146824 TEH Amount: 72.8791

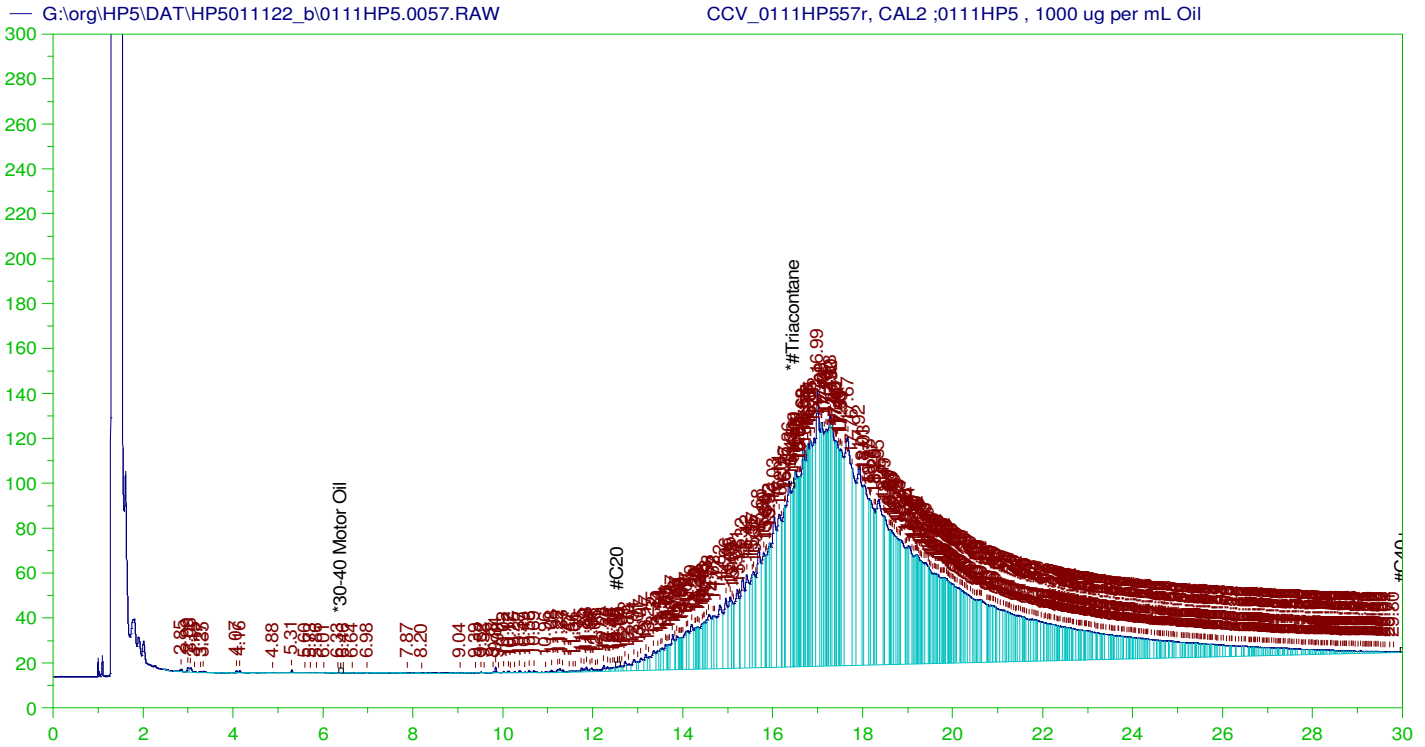

**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: CCV\_0111HP557r, CAL2 ;0111HP5 , 1000 ug per mL Oil  
 Raw File: G:\org\HP5\DAT\HP5011122\_b\0111HP5.0057.RAW  
 Date & Time Acquired: 1/13/2022 4:31:31 PM  
 Method File: G:\Org\HP5\Methods\DC\_ORO-57-BA-L\MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BA.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 26424.55  
 Rt range for Residual Range Organics: 12.51 to 30.05


SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*#Triacontane	16.454	500.	3.058	.61	-

RRO Area: 2.729502E+07 RRO AMOUNT: 1032.941

CONTINUING CALIBRATION REPORT: G:\org\HP5\DAT\HP5011122\_b\0111HP5.0057.RAW

COMPOUND	ACTUAL (NG)	MEASURED (NG)	%RECOVERY	LIMITS
*30-40 Motor Oil	5000.	.	75-125	

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	LIMITS
*#Triacontane	16.454	200.	3.058	1.53	75-125

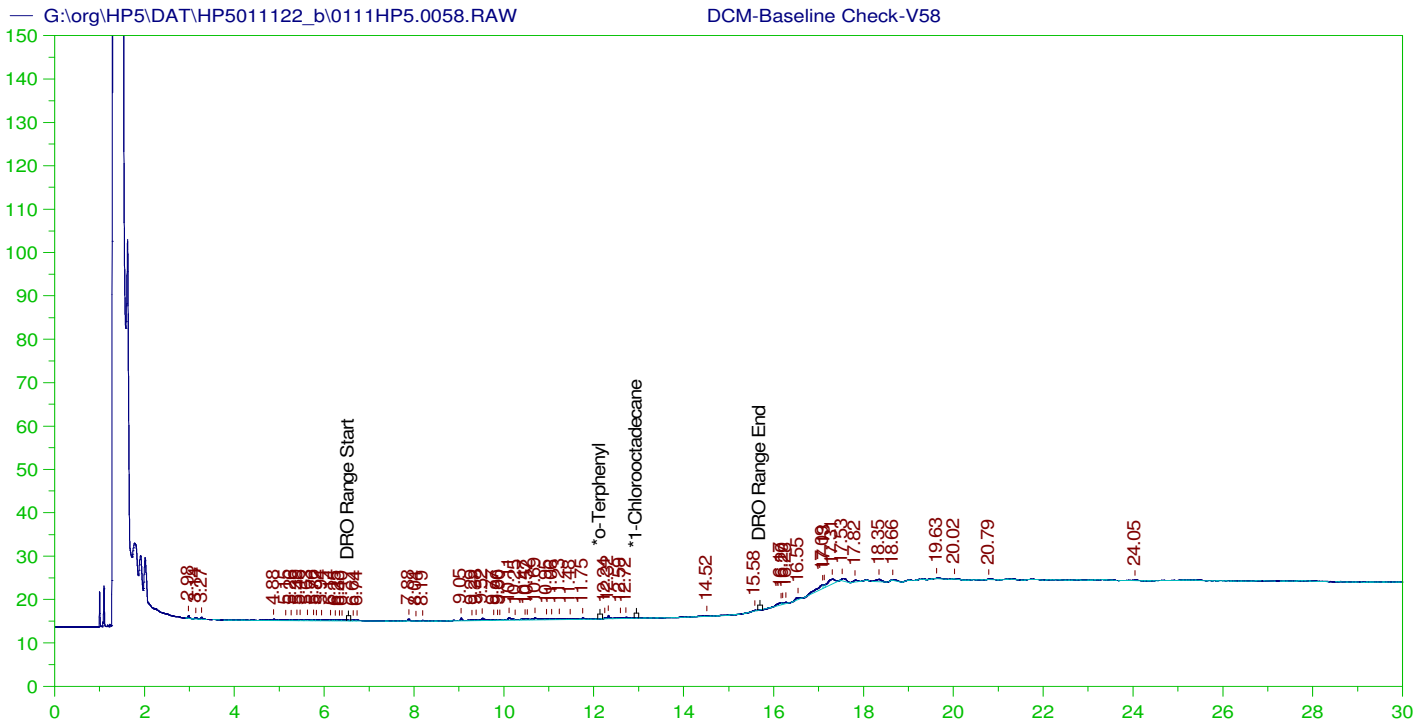

**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**


Sample Name: DCM-Baseline Check-V58  
 Raw File: G:\org\HP5\DAT\HP5011122\_b\0111HP5.0058.RAW  
 Date & Time Acquired: 1/13/2022 5:14:45 PM  
 Method File: G:\Org\HP5\Methods\DR\_8015-HE-LEXP.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO210108HE.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for TEH: 29457.33

Rt range for Diesel Range Organics: 6.49 to 15.75

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	29.94	200.	.	-
*1-Chlorooctadecane	29.94	200.	.	-

DRO Area:48306.73 DRO Amount: 1.639888  
 TEH Area:141285.5 TEH Amount: 4.796276



**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: CCV\_0111HP559r, CAL3 ;0111HP5 , 5000 ug per mL Oil  
 Raw File: G:\org\HP5\DAT\HP5011122\_b\0111HP5.0059.RAW  
 Date & Time Acquired: 1/13/2022 5:57:48 PM  
 Method File: G:\Org\HP5\Methods\DC\_ORO-59-BA-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BA.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 26424.55  
 Rt range for Residual Range Organics: 12.51 to 30.05


SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*#Triacontane	16.442	500.	33.09	6.62	-

RRO Area:1.303441E+08 RRO AMOUNT: 4932.688

CONTINUING CALIBRATION REPORT: G:\org\HP5\DAT\HP5011122\_b\0111HP5.0059.RAW

COMPOUND	ACTUAL (NG)	MEASURED (NG)	%RECOVERY	LIMITS
*30-40 Motor Oil	5000.	.037	.	75-125

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	LIMITS
*#Triacontane	16.442	200.	33.09	16.54	75-125



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: DCM-Baseline Check-V60  
 Raw File: G:\org\HP5\DAT\HP5011122\_b\0111HP5.0060.RAW  
 Date & Time Acquired: 1/13/2022 6:41:03 PM  
 Method File: G:\Org\HP5\Methods\DR\_8015-HE-LEXP.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO210108HE.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1


Mean RF for TEH: 29457.33

Rt range for Diesel Range Organics: 6.49 to 15.75

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	29.911	200.	.	-
*1-Chlorooctadecane	29.911	200.	.	-

DRO Area:316779.5 DRO Amount: 10.75384  
 TEH Area:980005.5 TEH Amount: 33.26864





**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: CCV\_0111HP561r, CAL4 ;0111HP5 , 15000 ug per mL Oil  
 Raw File: G:\org\HP5\DAT\HP5011122\_b\0111HP5.0061.RAW  
 Date & Time Acquired: 1/13/2022 7:24:16 PM  
 Method File: G:\Org\HP5\Methods\DC\_ORO-61-BA-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BA.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 26424.55  
 Rt range for Residual Range Organics: 12.51 to 30.05

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*#Triacontane	16.429	500.	33.728	6.75	-


RRO Area: 3.786286E+08 RRO AMOUNT: 14328.67

CONTINUING CALIBRATION REPORT: G:\org\HP5\DAT\HP5011122\_b\0111HP5.0061.RAW

COMPOUND	ACTUAL (NG)	MEASURED (NG)	%RECOVERY	LIMITS
*30-40 Motor Oil	5000.	.086	.	75-125

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	LIMITS
*#Triacontane	16.429	200.	33.728	16.86	75-125




**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: DCM-Baseline Check-V62  
 Raw File: G:\org\HP5\DAT\HP5011122\_b\0111HP5.0062.RAW  
 Date & Time Acquired: 1/13/2022 8:07:28 PM  
 Method File: G:\Org\HP5\Methods\DR\_8015-HE-LEXP.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO210108HE.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for TEH: 29457.33  
 Rt range for Diesel Range Organics: 6.49 to 15.75

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	29.883	200.	.	-
*1-Chlorooctadecane	29.883	200.	.	-

DRO Area:289041.4 DRO Amount: 9.812207  
 TEH Area:1408450 TEH Amount: 47.81323

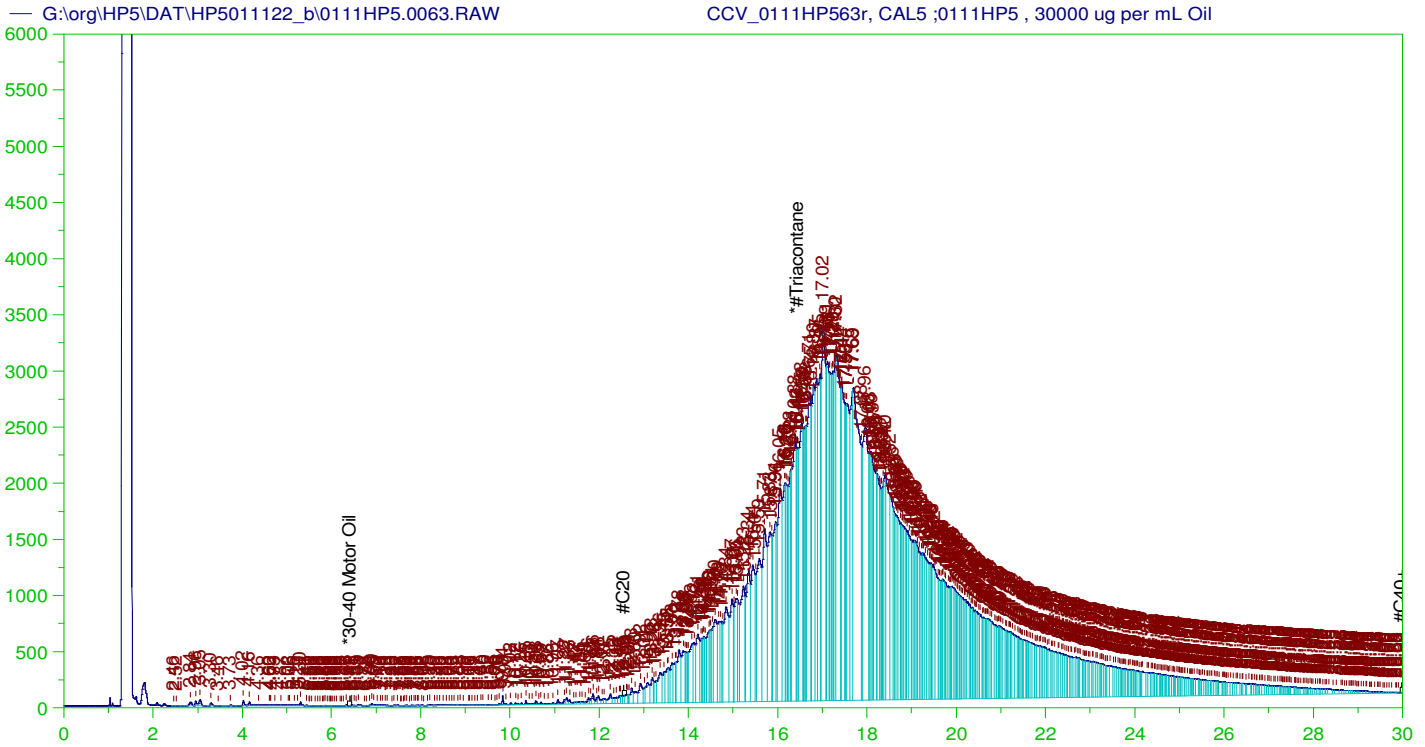

**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: CCV\_0111HP563r, CAL5 ;0111HP5 , 30000 ug per mL Oil  
 Raw File: G:\org\HP5\DAT\HP5011122\_b\0111HP5.0063.RAW  
 Date & Time Acquired: 1/13/2022 8:50:32 PM  
 Method File: G:\Org\HP5\Methods\DC\_ORO-BA-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BA.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 26424.55  
 Rt range for Residual Range Organics: 12.51 to 30.05


SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*#Triacontane	16.44	500.	102.625	20.52	-

RRO Area: 7.608009E+08 RRO AMOUNT: 28791.44

CONTINUING CALIBRATION REPORT: G:\org\HP5\DAT\HP5011122\_b\0111HP5.0063.RAW

COMPOUND	ACTUAL (NG)	MEASURED (NG)	%RECOVERY	LIMITS
*30-40 Motor Oil	5000.	.102	.	75-125

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	LIMITS
*#Triacontane	16.44	200.	102.625	51.31	75-125




**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: DCM-Baseline Check-V64  
 Raw File: G:\org\HP5\DAT\HP5011122\_b\0111HP5.0064.RAW  
 Date & Time Acquired: 1/13/2022 9:33:32 PM  
 Method File: G:\Org\HP5\Methods\DR\_8015-HE-LEXP.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO210108HE.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for TEH: 29457.33  
 Rt range for Diesel Range Organics: 6.49 to 15.75

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	29.741	200.	.	-
*1-Chlorooctadecane	29.741	200.	.	-

DRO Area:282237.4 DRO Amount: 9.581227  
 TEH Area:2669631 TEH Amount: 90.62704

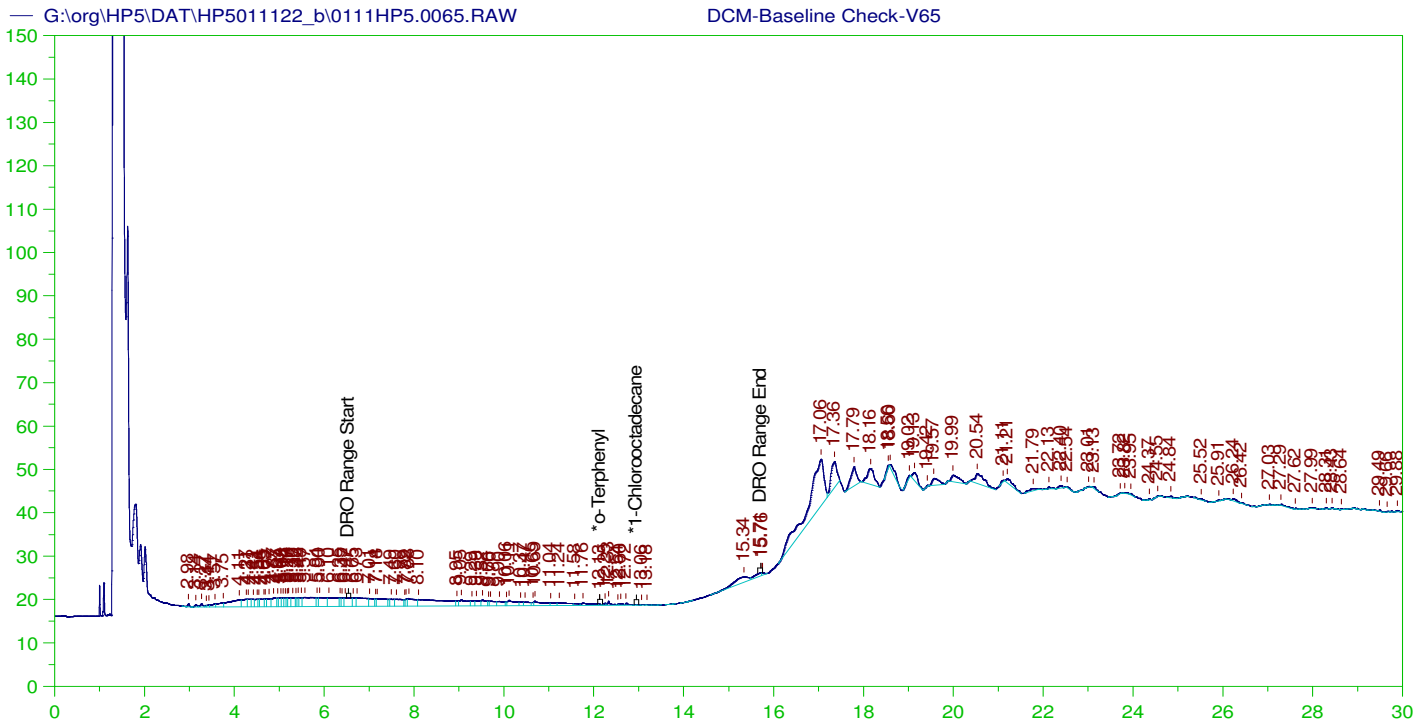

**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**


Sample Name: DCM-Baseline Check-V65  
 Raw File: G:\org\HP5\DAT\HP5011122\_b\0111HP5.0065.RAW  
 Date & Time Acquired: 1/13/2022 10:16:33 PM  
 Method File: G:\Org\HP5\Methods\DR\_8015-HE-LEXP.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO210108HE.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for TEH: 29457.33

Rt range for Diesel Range Organics: 6.49 to 15.75

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	12.129	200.	.021	.01
*1-Chlorooctadecane	29.884	200.	.	.

DRO Area:397141.5 DRO Amount: 13.48192  
 TEH Area:1310457 TEH Amount: 44.48662

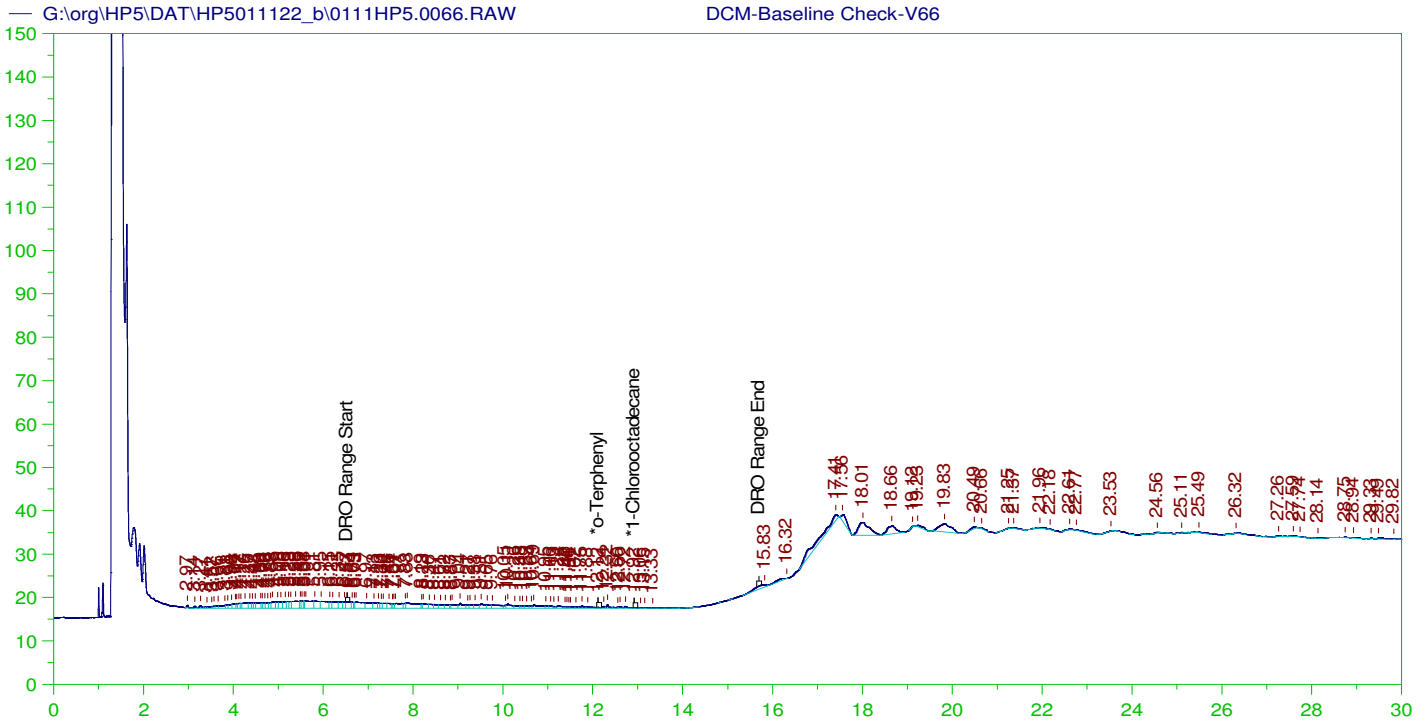


**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: DCM-Baseline Check-V66  
 Raw File: G:\org\HP5\DAT\HP5011122\_b\0111HP5.0066.RAW  
 Date & Time Acquired: 1/13/2022 10:59:39 PM  
 Method File: G:\Org\HP5\Methods\DR\_8015-HE-LEXP.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO210108HE.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for TEH: 29457.33  
 Rt range for Diesel Range Organics: 6.49 to 15.75

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	12.12	200.	.025	.01
*1-Chlorooctadecane	12.922	200.	.037	.02

DRO Area: 278500.4 DRO Amount: 9.454367  
 TEH Area: 757930.2 TEH Amount: 25.72976




**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: DCM-Baseline Check-V68  
 Raw File: G:\org\HP5\DAT\HP5011122\_b\0111HP5.0068.RAW  
 Date & Time Acquired: 1/14/2022 7:35:26 AM  
 Method File: G:\Org\HP5\Methods\DR\_8015-IC-LEXP.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO211102IC.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for TEH: 31353.19  
 Rt range for Diesel Range Organics: 6.5 to 15.82

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	29.833	200.	.	-
*1-Chlorooctadecane	29.833	200.	.	-

DRO Area:178261.1 DRO Amount: 5.685582  
 TEH Area:1513925 TEH Amount: 48.28614

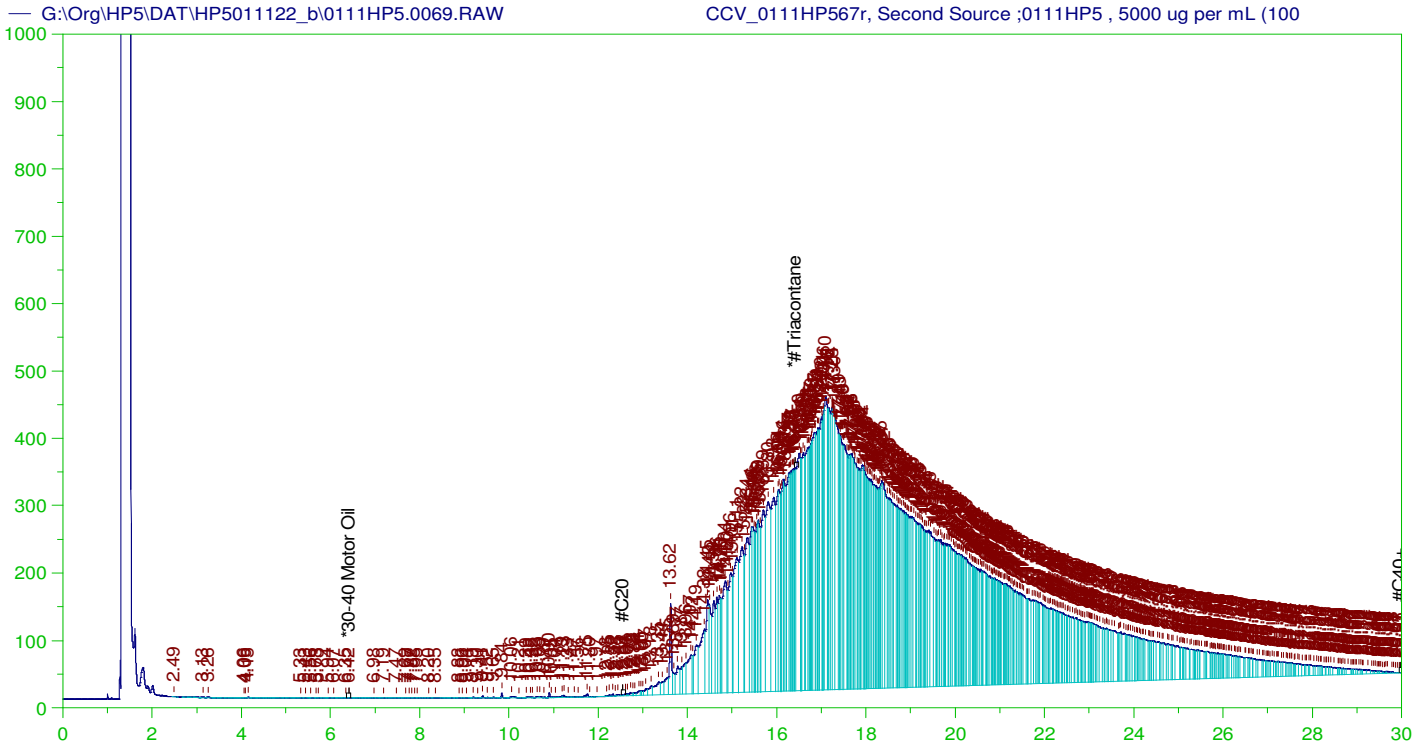

**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: CCV\_0111HP567r, Second Source ;0111HP5 , 5000 ug per mL (100  
 Raw File: G:\Org\HP5\DAT\HP5011122\_b\0111HP5.0069.RAW  
 Date & Time Acquired: 1/14/2022 8:18:14 AM  
 Method File: G:\Org\HP5\Methods\DC\_ORO-59-BA-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BA.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 26424.55  
 Rt range for Residual Range Organics: 12.51 to 30.05

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*#Triacontane_____	16.408	500.	23.958	4.79	-

RRO Area:1.341574E+08 RRO AMOUNT: 5076.999

CONTINUING CALIBRATION REPORT: G:\Org\HP5\DAT\HP5011122\_b\0111HP5.0069.RAW

COMPOUND	ACTUAL (NG)	MEASURED (NG)	%RECOVERY	LIMITS
*30-40 Motor Oil_____	5000.	.033	.	75-125

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	LIMITS
*#Triacontane_____	16.408	200.	23.958	11.98	75-125



Write Sequence	Data File	Sample Name	Method	Weight	Dil Factor	Amt Inj.	IS	Cal ID	Manual Integrations
	G:\org\HP5\DAT\HP5011122_b\0111HP5.25r	DCM-Baseline Check-V25	G:\Org\HP5\Methods\DR_8015-IC-LEXP.met	1	1	1	1	0	No Integrations
	G:\org\HP5\DAT\HP5011122_b\0111HP5.26r	Marker_0111HP526r_DRO_0111HP5 , DRO220111A	G:\org\HP5\Methods\CSC210212.met	1	1	1	1	0	No Integrations
	G:\org\HP5\DAT\HP5011122_b\0111HP5.27r	DCM-Baseline Check-V27	G:\Org\HP5\Methods\DR_8015-HS-LEXP.met	1	1	1	1	0	No Integrations
	G:\org\HP5\DAT\HP5011122_b\0111HP5.28r	CCV_0111HP528r, CAL1 :0111HP5 , 2 ug per mL Triacotane (10 uL of Cal3 + 990 uL DCM(14647)	G:\Org\HP5\Methods\DS_ORO-BA-L#.MET	1	1	1	1	0	Surrogates are integrated using a valley to valley integration Set Baseline All Valley on at 16.04 minutes.
	G:\org\HP5\DAT\HP5011122_b\0111HP5.29r	CCV_0111HP529r, CAL2 :0111HP5 , 50 ug per mL Triacotane (100 uL Cal4 + 900 uL of DCM(14647)	G:\Org\HP5\Methods\DS_ORO-BA-L#.MET	1	1	1	1	0	Surrogates are integrated using a valley to valley integration Set Baseline All Valley on at 16.04 minutes.
	G:\org\HP5\DAT\HP5011122_b\0111HP5.30r	CCV_0111HP530r, CAL3 :0111HP5 , 200 ug per mL Triacotane (100uL of Cal5 + 400 uL DCM(14647)	G:\Org\HP5\Methods\DS_ORO-BA-L#.MET	1	1	1	1	0	Surrogates are integrated using a valley to valley integration Set Baseline All Valley on at 16.04 minutes.
	G:\org\HP5\DAT\HP5011122_b\0111HP5.31r	CCV_0111HP531r, CAL4 :0111HP5 , 500 ug per mL Triacotane (250uL of Cal5 + 250 uL DCM(14647)	G:\Org\HP5\Methods\DS_ORO-BA-L#.MET	1	1	1	1	0	Surrogates are integrated using a valley to valley integration Set Baseline All Valley on at 16.04 minutes.
	G:\org\HP5\DAT\HP5011122_b\0111HP5.32r	DCM-Baseline Check-V33	G:\Org\HP5\Methods\DR_8015-HE-LEXP.met	1	1	1	1	0	No Integrations
	G:\org\HP5\DAT\HP5011122_b\0111HP5.50r	CCV_0111HP550r, CAL5 :0111HP5 , 1000 ug per mL Triacotane (DRO211006A)	G:\Org\HP5\Methods\DS_ORO-BA-L#.MET	1	1	1	1	0	Surrogates are integrated using a valley to valley integration Set Baseline All Valley on at 16.04 minutes.
	G:\org\HP5\DAT\HP5011122_b\0111HP5.51r	DCM-Baseline Check-V51	G:\Org\HP5\Methods\DR_8015-IC-LEXP.met	1	1	1	1	0	No Integrations
	G:\org\HP5\DAT\HP5011122_b\0111HP5.52r	DCM-Baseline Check-V52	G:\Org\HP5\Methods\DR_8015-IC-LEXP.met	1	1	1	1	0	No Integrations
	G:\org\HP5\DAT\HP5011122_b\0111HP5.53r	Marker_0111HP553r_DRO_0111HP5 , DRO220111A	G:\org\HP5\Methods\CSC210212.met	1	1	1	1	0	No Integrations
	G:\org\HP5\DAT\HP5011122_b\0111HP5.54r	DCM-Baseline Check-V54	G:\Org\HP5\Methods\DR_8015-IC-LEXP.met	1	1	1	1	0	No Integrations
	G:\org\HP5\DAT\HP5011122_b\0111HP5.55r	CCV_0111HP555r, CAL1 :0111HP5 , 150 ug per mL Oil (10 uL of Cal4 + 990 uL DCM(14647)	G:\Org\HP5\Methods\DC_ORO-55-BA-L%.xls	1	1	1	1	0	The integration of TEH(Oil Range)is the hydrocarbon response with reference to the baseline. Assigned Set Baseline Now at 25 minutes. Y-Scale adjusted.
	G:\org\HP5\DAT\HP5011122_b\0111HP5.56r	DCM-Baseline Check-V56	G:\Org\HP5\Methods\DR_8015-HE-LEXP.met	1	1	1	1	0	No Integrations
	G:\org\HP5\DAT\HP5011122_b\0111HP5.57r	CCV_0111HP557r, CAL2 :0111HP5 , 1000 ug per mL Oil (200 uL of Cal 3 +800 uL DCM(14647)	G:\Org\HP5\Methods\DC_ORO-57-BA-L%.xls	1	1	1	1	0	The integration of TEH(Oil Range)is the hydrocarbon response with reference to the baseline. Y-Scale adjusted.
	G:\org\HP5\DAT\HP5011122_b\0111HP5.58r	DCM-Baseline Check-V58	G:\Org\HP5\Methods\DR_8015-HE-LEXP.met	1	1	1	1	0	No Integrations
	G:\org\HP5\DAT\HP5011122_b\0111HP5.59r	CCV_0111HP559r, CAL3 :0111HP5 , 5000 ug per mL Oil (100 uL of DRO211118A + 900 uL DCM(14647)	G:\Org\HP5\Methods\DC_ORO-59-BA-L%.xls	1	1	1	1	0	The integration of TEH(Oil Range)is the hydrocarbon response with reference to the baseline. Y-Scale adjusted.
	G:\org\HP5\DAT\HP5011122_b\0111HP5.60r	DCM-Baseline Check-V60	G:\Org\HP5\Methods\DR_8015-HE-LEXP.met	1	1	1	1	0	No Integrations
	G:\org\HP5\DAT\HP5011122_b\0111HP5.61r	CCV_0111HP561r, CAL4 :0111HP5 , 15000 ug per mL Oil (200 uL of CAL5 + 200 uL DCM(14647)	G:\Org\HP5\Methods\DC_ORO-61-BA-L%.xls	1	1	1	1	0	The integration of TEH(Oil Range)is the hydrocarbon response with reference to the baseline. Y-Scale adjusted.
	G:\org\HP5\DAT\HP5011122_b\0111HP5.62r	DCM-Baseline Check-V62	G:\Org\HP5\Methods\DR_8015-HE-LEXP.met	1	1	1	1	0	No Integrations
	G:\org\HP5\DAT\HP5011122_b\0111HP5.63r	CCV_0111HP563r, CAL5 :0111HP5 , 30000 ug per mL Oil (600 uL of DRO211118A + 400 uL of DCM)	G:\Org\HP5\Methods\DC_ORO-BA-L%.xls	1	1	1	1	0	The integration of TEH(Oil Range)is the hydrocarbon response with reference to the baseline. Y-Scale adjusted.
	G:\org\HP5\DAT\HP5011122_b\0111HP5.64r	DCM-Baseline Check-V64	G:\Org\HP5\Methods\DR_8015-HE-LEXP.met	1	1	1	1	0	No Integrations
	G:\org\HP5\DAT\HP5011122_b\0111HP5.65r	DCM-Baseline Check-V65	G:\Org\HP5\Methods\DR_8015-HE-LEXP.met	1	1	1	1	0	No Integrations
	G:\org\HP5\DAT\HP5011122_b\0111HP5.66r	DCM-Baseline Check-V66	G:\Org\HP5\Methods\DR_8015-HE-LEXP.met	1	1	1	1	0	No Integrations
	G:\org\HP5\DAT\HP5011122_b\0111HP5.68r	DCM-Baseline Check-V68	G:\Org\HP5\Methods\DR_8015-IC-LEXP.met	1	1	1	1	0	No Integrations
	G:\org\HP5\DAT\HP5011122_b\0111HP5.69r	CCV_0111HP567r, Second Source :0111HP5 , 5000 ug per mL (100uL of DRO210902A + 900uL DCM(14647)	G:\Org\HP5\Methods\DC_ORO-59-BA-L%.xls	1	1	1	1	0	The integration of TEH(Oil Range)is the hydrocarbon response with reference to the baseline. Y-Scale adjusted.

*Ann Nebel*

Digitally signed by  
Ann Nebel  
Date: 2022.02.11 10:29:31 -07:00

# PREP BATCH REPORT

Prep Code: **HC-3520-DRO**  
 Prep Batch **163190** Prep Temp **NA °C**

Technician: **Jillian L Bostwick**  
 Batch Units: **ML**

Prep Start Date: **1/24/2022 3:16:21 PM**  
 Prep End Date: **1/25/2022 12:52:00 P**

Sample ID	Matrix	pH	Initial Samp Amt	Sol Added	Sol Recovered	Final Vol (mL)	Factor	Balance	Prep Start Date	Prep End Date
MB-163190			1000	0	0	1.00	0.001		1/24/2022	1/25/2022
Start time: 3:08 PM, 1/24/2022. End time: 01/25/2022 at 9:10 AM. SGT by ALN on remainder of sample on 1/26/2022.										
LCS-163190			1000	0	0	1.00	0.001		1/24/2022	1/25/2022
All bottles were completely used, defaced and disposed of on 1/24/2022.SGT by ALN on remainder of sample on 1/26/2022.										
LCSD-163190			1000	0	0	1.00	0.001		1/24/2022	1/25/2022
SGT by ALN on remainder of sample on 1/26/2022.										
LCS-163190-RRO			1000	0	0	1.00	0.001		1/24/2022	1/25/2022
SGT by ALN on remainder of sample on 1/27/2022.										
LCSD-163190-RRO			1000	0	0	1.00	0.001		1/24/2022	1/25/2022
SGT by ALN on remainder of sample on 1/27/2022.										
B22011446-001D	Ground Water	2	1010	0	0	1.00	0.00099		1/24/2022	1/25/2022
Bottle 1/2. Clear. SGT by ALN on remainder of sample on 1/27/2022.										
B22011446-001DMS	Ground Water	2	990	0	0	1.00	0.00101		1/24/2022	1/25/2022
Bottle 2/2. Clear. SGT by ALN on remainder of sample on 1/27/2022.										
B22011446-006D	Ground Water	2	990	0	0	1.00	0.00101		1/24/2022	1/25/2022
Bottle 1/2. Clear.SGT by ALN on remainder of sample on 1/26/2022.										
B22011446-006DMS-RRO	Ground Water	2	1060	0	0	1.00	0.000943		1/24/2022	1/25/2022
Bottle 2/2. Clear.SGT by ALN on remainder of sample on 1/26/2022.										
MDL2-163190-RRO			1000	0	0	1.00	0.001		1/24/2022	1/25/2022
SGT by ALN on remainder of sample on 1/26/2022.										
B22011446-011D	Ground Water	2	1010	0	0	1.00	0.00099		1/24/2022	1/25/2022
Bottle 1/2. Clear.SGT by ALN on remainder of sample on 1/26/2022.										
B22011446-012B	Ground Water	2	1030	0	0	1.00	0.000971		1/24/2022	1/25/2022
Bottle 1/2. Clear. SGT by ALN on remainder of sample on 1/26/2022.										
B22011446-017D	Ground Water	2	1030	0	0	1.00	0.000971		1/24/2022	1/25/2022
Bottle 1/2. Clear.SGT by ALN on remainder of sample on 1/26/2022.										
B22011446-022D	Ground Water	2	1020	0	0	1.00	0.00098		1/24/2022	1/25/2022
Bottle 1/2. Clear.SGT by ALN on remainder of sample on 1/26/2022.										

Number	Reagent Name	Exp Date
11	Carbon Filter Water	1/1/2023
13379	PTFE Boiling Stones 27463755	12/30/2025
14206	pH-indicator Strips 0-14 HC160347	8/26/2026
14719	4ML, Amber Vial, 20220104	1/4/2027
14747	Dichloromethane EC849	11/1/2023

Spk ID	Spike Name	SampType	AmtAdd	Exp Date
FP220120 14244	DCM RINSED FILTER PAPER	all	1	4/6/2026
Sulfate 01/18/22 (	Baked Sodium Sulfate	all	Varies	11/29/2026
DRO220119A	Triacotane SURR 1000 ug/mL	All except LCS, L	100 uL	4/6/2026
DRO211213A	OTP only SURR 2000 ug/mL	All except RRO-L	100 uL	9/30/2024
DRO220106C	#2 Diesel in Acetone 150,000 ug/mL	LCS, LCSD, MS,	100 uL	11/5/2023
DRO220112A	50,000 ug/mL Oil Std for RRO-In D	LCS-RRO, LCSD	100 uL	9/1/2026
DRO210902C	3,000 ug/mL Oil Std For MDLS-In D	MDL	100 uL	9/1/2026
DRO211006B	Triacotane SURR 20 ug/mL	MDL	100 uL	4/6/2026

# PREP BATCH REPORT

Prep Code: **HC-3520-DRO**  
 Prep Batch **163190** Prep Temp **NA °C**

Technician: **Jillian L Bostwick**  
 Batch Units: **ML**

Prep Start Date: **1/24/2022 3:16:21 PM**  
 Prep End Date: **1/25/2022 12:52:00 P**

Sample ID	Matrix	pH	Initial Samp Amt	Sol Added	Sol Recovered	Final Vol (mL)	Factor	Balance	Prep Start Date	Prep End Date
B22011446-027D	Ground Water	2	1040	0	0	1.00	0.000962		1/24/2022	1/25/2022
Bottle 1/2. Clear. SGT by ALN on remainder of sample on 1/27/2022.										
B22011446-032D	Ground Water	2	990	0	0	1.00	0.00101		1/24/2022	1/25/2022
Bottle 1/2. Clear.										

Number	Reagent Name	Exp Date
11	Carbon Filter Water	1/1/2023
13379	PTFE Boiling Stones 27463755	12/30/2025
14206	pH-indicator Strips 0-14 HC160347	8/26/2026
14719	4ML, Amber Vial, 20220104	1/4/2027
14747	Dichloromethane EC849	11/1/2023

Spk ID	Spike Name	SampType	AmtAdd	Exp Date
FP220120 14244	DCM RINSED FILTER PAPER	all	1	4/6/2026
Sulfate 01/18/22 (	Baked Sodium Sulfate	all	Varies	11/29/2026
DRO220119A	Triacontane SURR 1000 ug/mL	All except LCS, L	100 uL	4/6/2026
DRO211213A	OTP only SURR 2000 ug/mL	All except RRO-L	100 uL	9/30/2024
DRO220106C	#2 Diesel in Acetone 150,000 ug/mL	LCS, LCSD, MS,	100 uL	11/5/2023
DRO220112A	50,000 ug/mL Oil Std for RRO-In D	LCS-RRO, LCSD	100 uL	9/1/2026
DRO210902C	3,000 ug/mL Oil Std For MDLS-In D	MDL	100 uL	9/1/2026
DRO211006B	Triacontane SURR 20 ug/mL	MDL	100 uL	4/6/2026

# Energy Laboratories Inc

# ANALYTICAL RUN Summary

28-Jan-22

Run ID GCFID-HP5-B\_220124C

<b>Run Start Date:</b> 1/24/2022
<b>Analyst:</b> Ann Nebel
<b>Ical:</b>
<b>Column ID:</b>
<b>Comments:</b> DRO-8015-ICAL information is in Index GCFID-HP5-B_220111A 8015C OIL range calibration GCFID-HP5-B_220111C

Std ID	Std Name	Std Amount	Std Units	Samp Amount	Samp Units	SampType	Expiration Date
DRO220111A	Carbon Scan STD-Marker					MARKER	7/13/2026
DRO220118A	5,000 ug/mL RRO CCV 200 ug/mL Triacontane					CCV-RRO	4/6/2026
DRO220124A	8015 CCV-15,000ug/mL + 200 OTP					CCV-DRO	4/30/2023

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist						
14998892	CCV_0124HP55	HC-8015-DRO-	CCV		1/25/2022 9:31:5	1	R373715			0	0						
<b>Analyte</b>		<b>T</b>	<b>Units</b>	<b>RAW</b>	<b>Final</b>	<b>Text</b>	<b>Spike</b>	<b>SPKref</b>	<b>RPDref</b>	<b>MDL</b>	<b>PQL</b>	<b>UQL</b>	<b>%REC</b>	<b>LOW</b>	<b>HIGH</b>	<b>%RPD</b>	<b>Q</b>
TEH(Oil Range)		A	mg/L		4.42076123		5	0	0	0.0879	0.3	0	88%	80	120	0%	
n-Triacontane		S	mg/L		0.1980869		0.2	0	0	0.000336	0.002	0	99%	80	120	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist						
14998893	CCV_0124HP55	HC-8015-DRO-	CCV		1/25/2022 10:14:	1	R373715			0	0						
<b>Analyte</b>		<b>T</b>	<b>Units</b>	<b>RAW</b>	<b>Final</b>	<b>Text</b>	<b>Spike</b>	<b>SPKref</b>	<b>RPDref</b>	<b>MDL</b>	<b>PQL</b>	<b>UQL</b>	<b>%REC</b>	<b>LOW</b>	<b>HIGH</b>	<b>%RPD</b>	<b>Q</b>
Diesel Range Organics (C10 to C24)		A	mg/L		13.14187		15	0	0	0.0389	0.3	0	88%	80	120	0%	
Total Extractable Hydrocarbons		A	mg/L		13.5927		15	0	0	0.0749	0.3	50	91%	80	120	0%	
o-Terphenyl		S	mg/L		0.1800096		0.2	0	0	0.000429	0.002	0	90%	80	120	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist						
14998894	LCS-163190	HC-8015-DRO-	LCS-DOD		1/25/2022 11:40:	1	163190	1/24/2022 3:		0	0						
<b>Analyte</b>		<b>T</b>	<b>Units</b>	<b>RAW</b>	<b>Final</b>	<b>Text</b>	<b>Spike</b>	<b>SPKref</b>	<b>RPDref</b>	<b>MDL</b>	<b>PQL</b>	<b>UQL</b>	<b>%REC</b>	<b>LOW</b>	<b>HIGH</b>	<b>%RPD</b>	<b>Q</b>

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14998894	LCS-163190	HC-8015-DRO-	LCS-DOD		1/25/2022 11:40:	1	163190	1/24/2022 3:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Diesel Range Organics (C10 to C24)	A	mg/L		11.53646		15	0	0	0.0389	0.3	0	77%	36	132	0%	
Total Extractable Hydrocarbons	A	mg/L		12.33174		15	0	0	0.0749	0.3	50	82%	60	132	0%	
o-Terphenyl	S	mg/L		0.1757533		0.2	0	0	0.000429	0.002	0	88%	56	125	0%	
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14998895	LCSD-163190	HC-8015-DRO-	LCSD-DOD		1/26/2022 12:23:	1	163190	1/24/2022 3:	0	1E+07						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Diesel Range Organics (C10 to C24)	A	mg/L		11.40115		15	0	11.53646	0.0389	0.3	0	76%	36	132	1%	
Total Extractable Hydrocarbons	A	mg/L		12.20256		15	0	12.33174	0.0749	0.3	50	81%	60	132	1%	
o-Terphenyl	S	mg/L		0.1760508		0.2	0	0	0.000429	0.002	0	88%	56	125	0%	
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14998896	MB-163190	HC-8015-DRO-	MBLK		1/26/2022 1:05:5	1	163190	1/24/2022 3:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Diesel Range Organics (C10 to C24)	A	mg/L		0		0	0	0	0.0389	0.15	0	0%	0	0	0%	
Oil Range Hydrocarbons (C24 to C40)	A	mg/L		0		0	0	0	0.0879	0.15	0	0%	0	0	0%	
Total Extractable Hydrocarbons	A	mg/L		0		0	0	0	0.0749	0.15	50	0%	0	0	0%	
n-Triacontane	S	mg/L		0.096		0.1	0	0	0.000336	0.002	0	96%	50	150	0%	
o-Terphenyl	S	mg/L		0.190349		0.2	0	0	0.000429	0.002	0	95%	56	125	0%	
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14998897	B22011446-006	HC-8015-DRO-	SAMP		1/26/2022 1:48:3	1	163190	1/24/2022 3:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Diesel Range Organics (C10 to C24)	A	mg/L		0		0	0	0	0.039289	0.303	0	0%	0	0	0%	U
Oil Range Hydrocarbons (C24 to C40)	A	mg/L		0		0	0	0	0.088779	0.303	0	0%	0	0	0%	U
Total Extractable Hydrocarbons	A	mg/L		0		0	0	0	0.075649	0.303	50	0%	0	0	0%	U
n-Triacontane	S	mg/L		0.092		0.101	0	0	0.0003394	0.00202	0	91%	50	150	0%	
o-Terphenyl	S	mg/L		0.1814605		0.202	0	0	0.0004333	0.00202	0	90%	56	125	0%	
TEH(Oil Range)	X	mg/L		0		0	0	0	0.088779	0.303	0	0%	0	0	0%	U

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14998898	B22011446-017	HC-8015-DRO-	SAMP		1/26/2022 2:31:2	1	163190	1/24/2022 3:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Diesel Range Organics (C10 to C24)	A	mg/L		0.5906921		0	0	0	0.0377719	0.3	0	0%	0	0	0%	
Oil Range Hydrocarbons (C24 to C40)	A	mg/L		0.44308311		0	0	0	0.0853509	0.3	0	0%	0	0	0%	
Total Extractable Hydrocarbons	A	mg/L		1.010005		0	0	0	0.0727279	0.3	50	0%	0	0	0%	
n-Triacontane	S	mg/L		0.091		0.0971	0	0	0.0003263	0.001942	0	94%	50	150	0%	
o-Terphenyl	S	mg/L		0.1724877		0.1942	0	0	0.0004166	0.002	0	89%	56	125	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14998899	B22011446-022	HC-8015-DRO-	SAMP		1/26/2022 4:39:5	1	163190	1/24/2022 3:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Diesel Range Organics (C10 to C24)	A	mg/L		1.04066		0	0	0	0.038122	0.3	0	0%	0	0	0%	
Oil Range Hydrocarbons (C24 to C40)	A	mg/L		0.38294372		0	0	0	0.086142	0.3	0	0%	0	0	0%	
Total Extractable Hydrocarbons	A	mg/L		1.422858		0	0	0	0.073402	0.3	50	0%	0	0	0%	
n-Triacontane	S	mg/L		0.088		0.098	0	0	0.0003293	0.00196	0	90%	50	150	0%	
o-Terphenyl	S	mg/L		0.1714637		0.196	0	0	0.0004204	0.002	0	87%	56	125	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14998900	B22011446-012	HC-8015-DRO-	SAMP		1/26/2022 5:22:3	1	163190	1/24/2022 3:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Diesel Range Organics (C10 to C24)	A	mg/L		0.3731379		0	0	0	0.0377719	0.3	0	0%	0	0	0%	
Oil Range Hydrocarbons (C24 to C40)	A	mg/L		0.33518940		0	0	0	0.0853509	0.3	0	0%	0	0	0%	
Total Extractable Hydrocarbons	A	mg/L		0.7007675		0	0	0	0.0727279	0.3	50	0%	0	0	0%	
n-Triacontane	S	mg/L		0.094		0.0971	0	0	0.0003263	0.001942	0	97%	50	150	0%	
o-Terphenyl	S	mg/L		0.1724593		0.1942	0	0	0.0004166	0.002	0	89%	56	125	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14998901	B22011446-011	HC-8015-DRO-	SAMP		1/26/2022 6:05:2	1	163190	1/24/2022 3:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Diesel Range Organics (C10 to C24)	A	mg/L		0.3116207		0	0	0	0.038511	0.3	0	0%	0	0	0%	
Oil Range Hydrocarbons (C24 to C40)	A	mg/L		0.23697083		0	0	0	0.087021	0.3	0	0%	0	0	0%	J
Total Extractable Hydrocarbons	A	mg/L		0.580276		0	0	0	0.074151	0.3	50	0%	0	0	0%	
n-Triacontane	S	mg/L		0.092		0.099	0	0	0.0003326	0.00198	0	93%	50	150	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14998901	B22011446-011	HC-8015-DRO-	SAMP		1/26/2022 6:05:2	1	163190	1/24/2022 3:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
o-Terphenyl	S	mg/L		0.1204381		0.198	0	0	0.0004247	0.002	0	61%	56	125	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14998902	B22011446-032	HC-8015-DRO-	SAMP		1/26/2022 7:30:5	1	163190	1/24/2022 3:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Diesel Range Organics (C10 to C24)	A	mg/L		0		0	0	0	0.039289	0.303	0	0%	0	0	0%	U
Oil Range Hydrocarbons (C24 to C40)	A	mg/L		0		0	0	0	0.088779	0.303	0	0%	0	0	0%	U
Total Extractable Hydrocarbons	A	mg/L		0		0	0	0	0.075649	0.303	50	0%	0	0	0%	U
n-Triacontane	S	mg/L		0.088		0.101	0	0	0.0003394	0.00202	0	87%	50	150	0%	
o-Terphenyl	S	mg/L		0.1711838		0.202	0	0	0.0004333	0.00202	0	85%	56	125	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14998903	CCV_0124HP56	HC-8015-DRO-	CCV		1/26/2022 8:56:2	1	R373715				0	0				
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
TEH(Oil Range)	A	mg/L		4.55282471		5	0	0	0.0879	0.3	0	91%	80	120	0%	
n-Triacontane	S	mg/L		0.2044881		0.2	0	0	0.000336	0.002	0	102%	80	120	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
14998904	CCV_0124HP57	HC-8015-DRO-	CCV		1/26/2022 9:39:2	1	R373715				0	0				
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Diesel Range Organics (C10 to C24)	A	mg/L		13.00008		15	0	0	0.0389	0.3	0	87%	80	120	0%	
Total Extractable Hydrocarbons	A	mg/L		13.45098		15	0	0	0.0749	0.3	50	90%	80	120	0%	
o-Terphenyl	S	mg/L		0.1786011		0.2	0	0	0.000429	0.002	0	89%	80	120	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15001203	B22011446-001	HC-8015-DRO-	SAMP		1/26/2022 11:48:	1	163190	1/24/2022 3:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Diesel Range Organics (C10 to C24)	A	mg/L		0.04765976		0	0	0	0.038511	0.3	0	0%	0	0	0%	J
Oil Range Hydrocarbons (C24 to C40)	A	mg/L		0.16823752		0	0	0	0.087021	0.3	0	0%	0	0	0%	J
Total Extractable Hydrocarbons	A	mg/L		0.2262686		0	0	0	0.074151	0.3	50	0%	0	0	0%	J

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15001203	B22011446-001	HC-8015-DRO-	SAMP		1/26/2022 11:48:	1	163190	1/24/2022 3:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
n-Triacontane	S	mg/L		0.086		0.099	0	0	0.0003326	0.00198	0	87%	50	150	0%	
o-Terphenyl	S	mg/L		0.1655593		0.198	0	0	0.0004247	0.002	0	84%	56	125	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15001204	B22011446-027	HC-8015-DRO-	SAMP		1/26/2022 12:30:	1	163190	1/24/2022 3:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Diesel Range Organics (C10 to C24)	A	mg/L		0		0	0	0	0.0374218	0.3	0	0%	0	0	0%	U
Oil Range Hydrocarbons (C24 to C40)	A	mg/L		0		0	0	0	0.0845598	0.3	0	0%	0	0	0%	U
Total Extractable Hydrocarbons	A	mg/L		0		0	0	0	0.0720538	0.3	50	0%	0	0	0%	U
n-Triacontane	S	mg/L		0.086		0.0962	0	0	0.0003232	0.001924	0	89%	50	150	0%	
o-Terphenyl	S	mg/L		0.1718869		0.1924	0	0	0.0004127	0.002	0	89%	56	125	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15001205	B22011446-001	HC-8015-DRO-	MS-DOD		1/26/2022 1:13:3	1	163190	1/24/2022 3:	2E+07	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Diesel Range Organics (C10 to C24)	A	mg/L		13.19709		15.15	0.0476598	0	0.039289	0.303	0	87%	36	132	0%	
Total Extractable Hydrocarbons	A	mg/L		14.46475		15.15	0.2262686	0	0.075649	0.303	50	94%	60	132	0%	
o-Terphenyl	S	mg/L		0.1931067		0.202	0	0	0.0004333	0.00202	0	96%	56	125	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15001206	B22011446-006	HC-8015-DRO-	MS-DOD		1/26/2022 1:56:0	1	163190	1/24/2022 3:	1E+07	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
TEH(Oil Range)	A	mg/L		4.75068617		4.715	0	0	0.0828897	0.3	0	101%	41	113	0%	
n-Triacontane	S	mg/L		0.09		0.0943	0	0	0.0003168	0.002	0	95%	50	150	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15001207	LCS-163190-RR	HC-8015-DRO-	LCS-DOD		1/26/2022 3:21:1	1	163190	1/24/2022 3:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
TEH(Oil Range)	A	mg/L		5.01597118		5	0	0	0.0879	0.3	0	100%	41	113	0%	
n-Triacontane	S	mg/L		0.096		0.1	0	0	0.000336	0.002	0	96%	50	150	0%	



Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15001208	LCSD-163190-R	HC-8015-DRO-	LCSD-DOD		1/26/2022 4:46:2	1	163190	1/24/2022 3:	0	2E+07						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
TEH(Oil Range)	A	mg/L		4.93728161		5	0	5.0159712	0.0879	0.3	0	99%	41	113	2%	
n-Triacontane	S	mg/L		0.093		0.1	0	0	0.000336	0.002	0	93%	50	150	0%	
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15001209	CCV_0124HP58	HC-8015-DRO-	CCV		1/26/2022 6:12:4	1	R373715		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
TEH(Oil Range)	A	mg/L		4.62969775		5	0	0	0.0879	0.3	0	93%	80	120	0%	
n-Triacontane	S	mg/L		0.2025735		0.2	0	0	0.000336	0.002	0	101%	80	120	0%	
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15001210	CCV_0124HP58	HC-8015-DRO-	CCV		1/26/2022 6:55:4	1	R373715		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Diesel Range Organics (C10 to C24)	A	mg/L		13.52452		15	0	0	0.0389	0.3	0	90%	80	120	0%	
Total Extractable Hydrocarbons	A	mg/L		13.96399		15	0	0	0.0749	0.3	50	93%	80	120	0%	
o-Terphenyl	S	mg/L		0.1860448		0.2	0	0	0.000429	0.002	0	93%	80	120	0%	

# Energy Laboratories Inc

# ANALYTICAL RUN Summary

28-Jan-22

Run ID GCFID-HP5-B\_220127A

<b>Run Start Date:</b> 1/27/2022
<b>Analyst:</b> Ann Nebel
<b>Ical:</b>
<b>Column ID:</b>
<b>Comments:</b> DRO-8015-ICAL information is in Index GCFID-HP5-B_220111A 8015C OIL range calibration GCFID-HP5-B_220111C

Std ID	Std Name	Std Amount	Std Units	Samp Amount	Samp Units	SampType	Expiration Date
DRO220111A	Carbon Scan STD-Marker					MARKER	7/13/2026
DRO220118A	5,000 ug/mL RRO CCV 200 ug/mL Triacontane					CCV-RRO	4/6/2026
DRO220124A	8015 CCV-15,000ug/mL + 200 OTP					CCV-DRO	4/30/2023

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist				
15004065	CCV_0127HP50	HC-8015-DRO-	CCV		1/27/2022 10:41:	1	R373844			0	0				
<b>Analyte</b>		<b>T Units</b>	<b>RAW</b>	<b>Final</b>	<b>Text</b>	<b>Spike</b>	<b>SPKref</b>	<b>RPDref</b>	<b>MDL</b>	<b>PQL</b>	<b>UQL</b>	<b>%REC</b>	<b>LOW</b>	<b>HIGH</b>	<b>%RPD Q</b>
TEH(Oil Range)		A mg/L		4.55414746		5	0	0	0.0879	0.3	0	91%	80	120	0%
n-Triacontane		S mg/L		0.2052738		0.2	0	0	0.000336	0.002	0	103%	80	120	0%

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist				
15004066	CCV_0127HP50	HC-8015-DRO-	CCV		1/27/2022 11:24:	1	R373844			0	0				
<b>Analyte</b>		<b>T Units</b>	<b>RAW</b>	<b>Final</b>	<b>Text</b>	<b>Spike</b>	<b>SPKref</b>	<b>RPDref</b>	<b>MDL</b>	<b>PQL</b>	<b>UQL</b>	<b>%REC</b>	<b>LOW</b>	<b>HIGH</b>	<b>%RPD Q</b>
Diesel Range Organics (C10 to C24)		A mg/L		13.38394		15	0	0	0.0389	0.3	0	89%	80	120	0%
Total Extractable Hydrocarbons		A mg/L		13.85749		15	0	0	0.0749	0.3	50	92%	80	120	0%
o-Terphenyl		S mg/L		0.1840947		0.2	0	0	0.000429	0.002	0	92%	80	120	0%

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist				
15004067	MDL2-163190-	HC-8015-DRO-	MDL		1/27/2022 12:49:	1	163190	1/24/2022 3:			0	0			
<b>Analyte</b>		<b>T Units</b>	<b>RAW</b>	<b>Final</b>	<b>Text</b>	<b>Spike</b>	<b>SPKref</b>	<b>RPDref</b>	<b>MDL</b>	<b>PQL</b>	<b>UQL</b>	<b>%REC</b>	<b>LOW</b>	<b>HIGH</b>	<b>%RPD Q</b>

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15004067	MDL2-163190-	HC-8015-DRO-	MDL		1/27/2022 12:49:	1	163190	1/24/2022 3:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
TEH (SGT-Oil Range)	A	mg/L		0.28509280		0.3	0	0	0.0879	0.3	0	95%	60	140	0%	
TEH(Oil Range)	A	mg/L		0.28509280		0.3	0	0	0.0879	0.3	0	95%	60	140	0%	
n-Triacontane	S	mg/L		0.0014		0.002	0	0	0.000336	0.002	0	70%	50	150	0%	
n-Triacontane (SGT)	S	mg/L		0.0014		0.002	0	0	0.000336	0.002	0	70%	50	150	0%	
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15004068	LCS-163190	HC-8015-DRO-	LCS-DOD		1/27/2022 1:31:5	1	163190	1/24/2022 3:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Diesel Range Organics (SGT-C10 to	A	mg/L		11.04848		15	0	0	0.0389	0.3	0	74%	36	132	0%	
Total Extractable Hydrocarbons (SGT	A	mg/L		11.74941		15	0	0	0.0329	0.3	0	78%	60	132	0%	
o-Terphenyl (SGT)	S	mg/L		0.1765888		0.2	0	0	0.000429	0.002	0	88%	56	125	0%	
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15004069	LCSD-163190	HC-8015-DRO-	LCSD-DOD		1/27/2022 2:14:2	1	163190	1/24/2022 3:	0	2E+07						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Diesel Range Organics (SGT-C10 to	A	mg/L		10.88607		15	0	11.04848	0.0389	0.3	0	73%	36	132	1%	
Total Extractable Hydrocarbons (SGT	A	mg/L		11.54375		15	0	11.74941	0.0329	0.3	0	77%	60	132	2%	
o-Terphenyl (SGT)	S	mg/L		0.1800103		0.2	0	0	0.000429	0.002	0	90%	56	125	0%	
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15004070	MB-163190	HC-8015-DRO-	MBLK		1/27/2022 2:56:5	1	163190	1/24/2022 3:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Diesel Range Organics (SGT-C10 to	A	mg/L		0		0	0	0	0.0389	0.15	0	0%	0	0	0%	
Oil Range Hydrocarbons (SGT-C24 t	A	mg/L		0		0	0	0	0.0879	0.15	0	0%	0	0	0%	
Total Extractable Hydrocarbons (SGT	A	mg/L		0		0	0	0	0.0329	0.15	0	0%	0	0	0%	
n-Triacontane (SGT)	S	mg/L		0.088		0.1	0	0	0.000336	0.002	0	88%	50	150	0%	
o-Terphenyl (SGT)	S	mg/L		0.1823085		0.2	0	0	0.000429	0.002	0	91%	56	125	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15004071	B22011446-006	HC-8015-DRO-	SAMP		1/27/2022 3:39:1	1	163190	1/24/2022 3:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Diesel Range Organics (SGT-C10 to	A	mg/L		0		0	0	0	0.039289	0.303	0	0%	0	0	0%	U
Oil Range Hydrocarbons (SGT-C24 t	A	mg/L		0		0	0	0	0.088779	0.303	0	0%	0	0	0%	U
Total Extractable Hydrocarbons (SGT	A	mg/L		0		0	0	0	0.033229	0.303	0	0%	0	0	0%	U
n-Triacontane (SGT)	S	mg/L		0.087		0.101	0	0	0.0003394	0.00202	0	86%	50	150	0%	
o-Terphenyl (SGT)	S	mg/L		0.1753322		0.202	0	0	0.0004333	0.00202	0	87%	56	125	0%	
TEH (SGT-Oil Range)	X	mg/L		0		0	0	0	0.088779	0.303	0	0%	0	0	0%	U

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15004072	B22011446-001	HC-8015-DRO-	SAMP		1/27/2022 4:21:3	1	163190	1/24/2022 3:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Diesel Range Organics (SGT-C10 to	A	mg/L		0		0	0	0	0.038511	0.3	0	0%	0	0	0%	U
Oil Range Hydrocarbons (SGT-C24 t	A	mg/L		0		0	0	0	0.087021	0.3	0	0%	0	0	0%	U
Total Extractable Hydrocarbons (SGT	A	mg/L		0		0	0	0	0.032571	0.3	0	0%	0	0	0%	U
n-Triacontane (SGT)	S	mg/L		0.085		0.099	0	0	0.0003326	0.00198	0	86%	50	150	0%	
o-Terphenyl (SGT)	S	mg/L		0.1705753		0.198	0	0	0.0004247	0.00198	0	86%	56	125	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15004073	B22011446-017	HC-8015-DRO-	SAMP		1/27/2022 5:04:1	1	163190	1/24/2022 3:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Diesel Range Organics (SGT-C10 to	A	mg/L		0		0	0	0	0.0377719	0.3	0	0%	0	0	0%	U
Oil Range Hydrocarbons (SGT-C24 t	A	mg/L		0		0	0	0	0.0853509	0.3	0	0%	0	0	0%	U
Total Extractable Hydrocarbons (SGT	A	mg/L		0.03276548		0	0	0	0.0319459	0.3	0	0%	0	0	0%	J
n-Triacontane (SGT)	S	mg/L		0.086		0.0971	0	0	0.0003263	0.001942	0	89%	50	150	0%	
o-Terphenyl (SGT)	S	mg/L		0.1812307		0.1942	0	0	0.0004166	0.001942	0	93%	56	125	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15004074	B22011446-022	HC-8015-DRO-	SAMP		1/27/2022 6:29:4	1	163190	1/24/2022 3:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Diesel Range Organics (SGT-C10 to	A	mg/L		0.6579801		0	0	0	0.038122	0.3	0	0%	0	0	0%	
Oil Range Hydrocarbons (SGT-C24 t	A	mg/L		0.12701969		0	0	0	0.086142	0.3	0	0%	0	0	0%	J
Total Extractable Hydrocarbons (SGT	A	mg/L		0.791407		0	0	0	0.032242	0.3	0	0%	0	0	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15004074	B22011446-022	HC-8015-DRO-	SAMP		1/27/2022 6:29:4	1	163190	1/24/2022 3:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
n-Triacontane (SGT)	S	mg/L		0.087		0.098	0	0	0.0003293	0.00196	0	89%	50	150	0%	
o-Terphenyl (SGT)	S	mg/L		0.1783509		0.196	0	0	0.0004204	0.00196	0	91%	56	125	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15004075	B22011446-012	HC-8015-DRO-	SAMP		1/27/2022 7:12:3	1	163190	1/24/2022 3:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Diesel Range Organics (SGT-C10 to	A	mg/L		0.07441181		0	0	0	0.0377719	0.3	0	0%	0	0	0%	J
Oil Range Hydrocarbons (SGT-C24 t	A	mg/L		0.12234417		0	0	0	0.0853509	0.3	0	0%	0	0	0%	J
Total Extractable Hydrocarbons (SGT	A	mg/L		0.20173		0	0	0	0.0319459	0.3	0	0%	0	0	0%	J
n-Triacontane (SGT)	S	mg/L		0.085		0.0971	0	0	0.0003263	0.001942	0	88%	50	150	0%	
o-Terphenyl (SGT)	S	mg/L		0.1687932		0.1942	0	0	0.0004166	0.001942	0	87%	56	125	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15004076	B22011446-011	HC-8015-DRO-	SAMP		1/27/2022 7:55:1	1	163190	1/24/2022 3:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Diesel Range Organics (SGT-C10 to	A	mg/L		0.07396293		0	0	0	0.038511	0.3	0	0%	0	0	0%	J
Oil Range Hydrocarbons (SGT-C24 t	A	mg/L		0		0	0	0	0.087021	0.3	0	0%	0	0	0%	U
Total Extractable Hydrocarbons (SGT	A	mg/L		0.1489561		0	0	0	0.032571	0.3	0	0%	0	0	0%	J
n-Triacontane (SGT)	S	mg/L		0.098		0.099	0	0	0.0003326	0.00198	0	99%	50	150	0%	
o-Terphenyl (SGT)	S	mg/L		0.1326084		0.198	0	0	0.0004247	0.00198	0	67%	56	125	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15004077	CCV_0127HP51	HC-8015-DRO-	CCV		1/27/2022 9:20:3	1	R373844				0	0				
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
TEH(Oil Range)	A	mg/L		4.62119287		5	0	0	0.0879	0.3	0	92%	80	120	0%	
n-Triacontane	S	mg/L		0.2117619		0.2	0	0	0.000336	0.002	0	106%	80	120	0%	

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15004078	CCV_0127HP52	HC-8015-DRO-	CCV		1/27/2022 10:03:	1	R373844				0	0				
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q

Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15004078	CCV_0127HP52	HC-8015-DRO-	CCV		1/27/2022 10:03:	1	R373844		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Diesel Range Organics (C10 to C24)	A	mg/L		14.08529		15	0	0	0.0389	0.3	0	94%	80	120	0%	
Total Extractable Hydrocarbons	A	mg/L		14.58281		15	0	0	0.0749	0.3	50	97%	80	120	0%	
o-Terphenyl	S	mg/L		0.1931111		0.2	0	0	0.000429	0.002	0	97%	80	120	0%	
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15004079	B22011446-001	HC-8015-DRO-	MS-DOD		1/28/2022 12:11:	1	163190	1/24/2022 3:	2E+07	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Diesel Range Organics (SGT-C10 to	A	mg/L		11.73847		15.15	0	0	0.039289	0.303	0	77%	36	132	0%	
Total Extractable Hydrocarbons (SGT	A	mg/L		12.54474		15.15	0	0	0.033229	0.303	0	83%	60	132	0%	
o-Terphenyl (SGT)	S	mg/L		0.1820785		0.202	0	0	0.0004333	0.00202	0	90%	56	125	0%	
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15004080	B22011446-006	HC-8015-DRO-	MS-DOD		1/28/2022 12:54:	1	163190	1/24/2022 3:	2E+07	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
TEH (SGT-Oil Range)	A	mg/L		4.32221889		4.715	0	0	0.0828897	0.3	0	92%	41	113	0%	
n-Triacontane (SGT)	S	mg/L		0.078		0.0943	0	0	0.0003168	0.002	0	83%	50	150	0%	
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15004081	LCS-163190-RR	HC-8015-DRO-	LCS-DOD		1/28/2022 2:19:1	1	163190	1/24/2022 3:	0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
TEH (SGT-Oil Range)	A	mg/L		4.99884892		5	0	0	0.0879	0.3	0	100%	41	113	0%	
n-Triacontane (SGT)	S	mg/L		0.094		0.1	0	0	0.000336	0.002	0	94%	50	150	0%	
Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15004082	LCSD-163190-R	HC-8015-DRO-	LCSD-DOD		1/28/2022 3:44:2	1	163190	1/24/2022 3:	0	2E+07						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
TEH (SGT-Oil Range)	A	mg/L		4.89216995		5	0	4.9988489	0.0879	0.3	0	98%	41	113	2%	
n-Triacontane (SGT)	S	mg/L		0.091		0.1	0	0	0.000336	0.002	0	91%	50	150	0%	


Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15004083	CCV_0127HP53	HC-8015-DRO-	CCV		1/28/2022 5:09:4	1	R373844		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
TEH(Oil Range)	A	mg/L		4.87059375		5	0	0	0.0879	0.3	0	97%	80	120	0%	
n-Triacontane	S	mg/L		0.2185442		0.2	0	0	0.000336	0.002	0	109%	80	120	0%	


Seq No	Lab ID	Test Code	Sample Typ	File ID	Analysis Date	DF	Batch ID	Prep Date	SPKref	RPDref	pmoist					
15004084	CCV_0127HP53	HC-8015-DRO-	CCV		1/28/2022 5:52:2	1	R373844		0	0						
Analyte	T	Units	RAW	Final	Text	Spike	SPKref	RPDref	MDL	PQL	UQL	%REC	LOW	HIGH	%RPD	Q
Diesel Range Organics (C10 to C24)	A	mg/L		13.38672		15	0	0	0.0389	0.3	0	89%	80	120	0%	
Total Extractable Hydrocarbons	A	mg/L		13.85663		15	0	0	0.0749	0.3	50	92%	80	120	0%	
o-Terphenyl	S	mg/L		0.18374		0.2	0	0	0.000429	0.002	0	92%	80	120	0%	





Write Sequence	Data File	Sample Name	Method	Weight	Dil Factor	Amt Inj.	IS	Cal ID
	G:\org\HP5\DAT\HP5012722_b\0127HP5.01r	DCM-Baseline Check-V01	G:\Org\HP5\Methods\DR_8015-JA-LEXP.met	1	1	1	1	0
	G:\org\HP5\DAT\HP5012722_b\0127HP5.02r	DCM-Baseline Check-V02	G:\Org\HP5\Methods\DR_8015-JA-LEXP.met	1	1	1	1	0
	G:\org\HP5\DAT\HP5012722_b\0127HP5.03r	MARKER_0127HP503r_DRO_0127HP5 , DRO220111A	G:\org\HP5\Methods\CSC220127.met	1	1	1	1	0
	G:\org\HP5\DAT\HP5012722_b\0127HP5.04r	CCV_0127HP504r_RRO_0127HP5 , DRO220118A	G:\Org\HP5\Methods\DC_ORO-BD-L%.MET G:\Org\HP5\Methods\DS_ORO-BD-L%.MET	1	1	1	1	0
	G:\org\HP5\DAT\HP5012722_b\0127HP5.05r	CCV_0127HP505r_DRO_0127HP5 , DRO220124A	G:\Org\HP5\Methods\DC_8015-C24-JD-L%.met G:\Org\HP5\Methods\DS_8015-C24-JD-L%.met	1	1	1	1	0
	G:\org\HP5\DAT\HP5012722_b\0127HP5.06r	DCM-Baseline Check-V05	G:\Org\HP5\Methods\DR_8015-JA-LEXP.met	1	1	1	1	0
	G:\org\HP5\DAT\HP5012722_b\0127HP5.08r	LCS-163190_0127HP5 , SGT	G:\Org\HP5\Methods\D3_8015-C24-JD-L%.met G:\Org\HP5\Methods\DS_8015-C24-JD-L%.met	1000	1	1	1	0
	G:\org\HP5\DAT\HP5012722_b\0127HP5.09r	LCSD-163190_0127HP5 , SGT	G:\Org\HP5\Methods\D3_8015-C24-JD-L%.met G:\Org\HP5\Methods\DS_8015-C24-JD-L%.met	1000	1	1	1	0
	G:\org\HP5\DAT\HP5012722_b\0127HP5.10r	MB-163190_0127HP5 , SGT	G:\Org\HP5\Methods\DR_8015-C24T-JD-L%.met G:\Org\HP5\Methods\DR_OROS-BD-L%.MET G:\Org\HP5\Methods\DS_8015-C24T-JD-L%.met	1000	1	1	1	0
	G:\org\HP5\DAT\HP5012722_b\0127HP5.11r	B22011446-006D_0127HP5 , \$HC-8015-DRO-W, SGT	G:\Org\HP5\Methods\DR_8015-C24T-JD-L%.met G:\Org\HP5\Methods\DR_OROS-BD-L%.MET G:\Org\HP5\Methods\DS_8015-C24T-JD-L%.met	990	1	1	1	0
	G:\org\HP5\DAT\HP5012722_b\0127HP5.12r	B22011446-001D_0127HP5 , \$HC-8015-DRO-W, SGT	G:\Org\HP5\Methods\DR_8015-C24T-JD-L%.met G:\Org\HP5\Methods\DR_OROS-BD-L%.MET G:\Org\HP5\Methods\DS_8015-C24T-JD-L%.met	1010	1	1	1	0
	G:\org\HP5\DAT\HP5012722_b\0127HP5.13r	B22011446-017D_0127HP5 , \$HC-8015-DRO-W, SGT	G:\Org\HP5\Methods\DR_8015-C24T-JD-L%.met G:\Org\HP5\Methods\DR_OROS-BD-L%.MET G:\Org\HP5\Methods\DS_8015-C24T-JD-L%.met	1030	1	1	1	0
	G:\org\HP5\DAT\HP5012722_b\0127HP5.14r	DCM-Baseline Check-V14	G:\Org\HP5\Methods\DR_8015-JA-LEXP.met	1	1	1	1	0
	G:\org\HP5\DAT\HP5012722_b\0127HP5.15r	B22011446-022D_0127HP5 , \$HC-8015-DRO-W, SGT	G:\Org\HP5\Methods\D3_8015-C24T-JD-L%.met G:\Org\HP5\Methods\D3_OROS-BD-L%.MET G:\Org\HP5\Methods\DS_8015-C24T-JD-L%.met	1020	1	1	1	0
	G:\org\HP5\DAT\HP5012722_b\0127HP5.16r	B22011446-012B_0127HP5 , \$HC-8015-DRO-W, SGT	G:\Org\HP5\Methods\D3_8015-012716-JD-L%.met G:\Org\HP5\Methods\D3_OROS-012716-BD-L%.MET G:\Org\HP5\Methods\DS_8015-C24T-JD-L%.met	1030	1	1	1	0
	G:\org\HP5\DAT\HP5012722_b\0127HP5.17r	B22011446-011D_0127HP5 , \$HC-8015-DRO-W, SGT	G:\Org\HP5\Methods\DR_8015-012717-JD-L%.met G:\Org\HP5\Methods\D3_OROS-012717-BD-L%.MET G:\Org\HP5\Methods\DS_8015-C24T-JD-L%.met	1010	1	1	1	0
	G:\org\HP5\DAT\HP5012722_b\0127HP5.18r	MARKER_0127HP518r_DRO_0127HP5 , DRO220111A	G:\org\HP5\Methods\CSC220127.met	1	1	1	1	0
	G:\org\HP5\DAT\HP5012722_b\0127HP5.19r	CCV_0127HP519r_RRO_0127HP5 , DRO220118A	G:\Org\HP5\Methods\DC_ORO-BD-L%.MET G:\Org\HP5\Methods\DS_ORO-BD-L%.MET	1	1	1	1	0
	G:\org\HP5\DAT\HP5012722_b\0127HP5.20r	CCV_0127HP520r_DRO_0127HP5 , DRO220124A	G:\Org\HP5\Methods\DC_8015-C24-JD-L%.met G:\Org\HP5\Methods\DS_8015-C24-JD-L%.met	1	1	1	1	0
	G:\org\HP5\DAT\HP5012722_b\0127HP5.21r	DCM-Baseline Check-V21	G:\Org\HP5\Methods\DR_8015-JA-LEXP.met	1	1	1	1	0
	G:\org\HP5\DAT\HP5012722_b\0127HP5.22r	DCM-Baseline Check-V22	G:\Org\HP5\Methods\DR_8015-JA-LEXP.met	1	1	1	1	0
	G:\org\HP5\DAT\HP5012722_b\0127HP5.23r	B22011446-001DMS_0127HP5 , SGT	G:\Org\HP5\Methods\D3_8015-C24-JD-L%.met G:\Org\HP5\Methods\DS_8015-C24-JD-L%.met	990	1	1	1	0
	G:\org\HP5\DAT\HP5012722_b\0127HP5.24r	B22011446-006DMS-RRO_0127HP5 , SGT	G:\Org\HP5\Methods\D3_ORO-BD-L%.MET G:\Org\HP5\Methods\DS_ORO-BD-L%.MET	1060	1	1	1	0
	G:\org\HP5\DAT\HP5012722_b\0127HP5.25r	DCM-Baseline Check-V25	G:\Org\HP5\Methods\DR_8015-JA-LEXP.met	1	1	1	1	0
	G:\org\HP5\DAT\HP5012722_b\0127HP5.26r	LCS-163190-RRO_0127HP5 , SGT	G:\Org\HP5\Methods\D3_ORO-BD-L%.MET G:\Org\HP5\Methods\DS_ORO-BD-L%.MET	1000	1	1	1	0
	G:\org\HP5\DAT\HP5012722_b\0127HP5.27r	DCM-Baseline Check-V27	G:\Org\HP5\Methods\DR_8015-JA-LEXP.met	1	1	1	1	0
	G:\org\HP5\DAT\HP5012722_b\0127HP5.28r	LCSD-163190-RRO_0127HP5 , SGT	G:\Org\HP5\Methods\D3_ORO-BD-L%.MET G:\Org\HP5\Methods\DS_ORO-BD-L%.MET	1000	1	1	1	0
	G:\org\HP5\DAT\HP5012722_b\0127HP5.29r	MARKER_0127HP529r_DRO_0127HP5 , DRO220111A	G:\org\HP5\Methods\CSC220127.met	1	1	1	1	0
	G:\org\HP5\DAT\HP5012722_b\0127HP5.30r	CCV_0127HP530r_RRO_0127HP5 , DRO220118A	G:\Org\HP5\Methods\DC_ORO-BD-L%.MET G:\Org\HP5\Methods\DS_ORO-BD-L%.MET	1	1	1	1	0
	G:\org\HP5\DAT\HP5012722_b\0127HP5.31r	CCV_0127HP531r_DRO_0127HP5 , DRO220124A	G:\Org\HP5\Methods\DC_8015-C24-JD-L%.met G:\Org\HP5\Methods\DS_8015-C24-JD-L%.met	1	1	1	1	0





**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: CCV\_0124HP553r, RRO ;0124HP5 , DRO220118A  
 Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0053.RAW  
 Date & Time Acquired: 1/25/2022 9:31:52 PM  
 Method File: G:\Org\HP5\Methods\DC\_ORO-BC-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BC.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for for ~~Residual~~ TEH(Oil Range) Organics Calculations: 26424.55  
 Rt range for ~~Residual~~ TEH(Oil Range) Organics: 12.65 to 30.05

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*#Triacontane	16.39	500.	317.866	63.57	-


~~RRO~~ TEH(Oil Range) Area:1.168166E+08 ~~RRO~~ TEH(Oil Range) AMOUNT: 4420.761

CONTINUING CALIBRATION REPORT: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0053.RAW

COMPOUND	ACTUAL (NG)	MEASURED (NG)	%RECOVERY	LIMITS
*30-40 Motor Oil	5000.	.151	.	75-125

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	LIMITS
*#Triacontane	16.39	200.	317.866	158.93	75-125

AMN 02/15/2022



**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: CCV\_0124HP553r, RRO ;0124HP5 , DRO220118A  
 Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0053.RAW  
 Date & Time Acquired: 1/25/2022 9:31:52 PM  
 Method File: G:\Org\HP5\Methods\DS\_ORO-BC-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BC.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 26424.55  
 Rt range for Residual Range Organics: 12.65 to 30.05


SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*#Triacontane	16.39	500.	198.087	39.62	-

RRO Area:2989965 RRO AMOUNT: 113.151

CONTINUING CALIBRATION REPORT: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0053.RAW

COMPOUND	ACTUAL (NG)	MEASURED (NG)	%RECOVERY	LIMITS
*30-40 Motor Oil	5000.	.151	.	75-125

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	LIMITS
*#Triacontane	16.39	200.	198.087	99.04	75-125



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: CCV\_0124HP554r, DRO ;0124HP5 , DRO220124A  
 Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0054.RAW  
 Date & Time Acquired: 1/25/2022 10:14:31 PM  
 Method File: G:\Org\HP5\Methods\DC\_8015-C24-JC-L%.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JC-C24.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36  
 Rt range for Diesel Range Organics: 6.58 to 14.47

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.307	200.	293.495	146.75	-
*1-Chlorooctadecane	13.154	200.	140.825	70.41	-

DRO Area: 4.294152E+08 DRO Amount: 13141.87  
 TEH Area: 4.441462E+08 TEH Amount: 13592.7


CONTINUING CALIBRATION REPORT: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0054.RAW

COMPOUND	ACTUAL (NG)	MEASURED (NG)	%RECOVERY	LIMITS
TOTAL DRO	15000.	13592.7	90.62	85-115

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	LIMITS
*o-Terphenyl	12.307	200.	293.495	146.75	85-115
*1-Chlorooctadecane	13.154	200.	140.825	70.41	85-115

G:\org\HP5\DAT\HP5012422\_b\0124HP5.0054.RAW

CCV\_0124HP54r, DRO ;0124HP5 , DRO220124A



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: CCV\_0124HP54r, DRO ;0124HP5 , DRO220124A  
 Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0054.RAW  
 Date & Time Acquired: 1/25/2022 10:14:31 PM  
 Method File: G:\Org\HP5\Methods\DS\_8015-C24-JC-L#.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JC-C24.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.58 to 14.47


SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	12.307	200.	180.01	90.
*1-Chlorooctadecane	13.154	200.	32.384	16.19

DRO Area: 2.215508E+08 DRO Amount: 6780.362  
 TEH Area: 2.312515E+08 TEH Amount: 7077.244

CONTINUING CALIBRATION REPORT: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0054.RAW

COMPOUND	ACTUAL (NG)	MEASURED (NG)	%RECOVERY	LIMITS
TOTAL DRO	15000.	7077.24	47.18	85-115

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	LIMITS
*o-Terphenyl	12.307	200.	180.01	90.	85-115
*1-Chlorooctadecane	13.154	200.	32.384	16.19	85-115



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: DCM-Baseline Check-V54  
 Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0055.RAW  
 Date & Time Acquired: 1/25/2022 10:57:22 PM  
 Method File: G:\Org\HP5\Methods\DR\_8015-JA-LEXP.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JA.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36  
 Rt range for Diesel Range Organics: 6.63 to 15.99


SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	29.906	200.	.	-
*1-Chlorooctadecane	29.906	200.	.	-

DRO Area:137830 DRO Amount: 4.218164  
 TEH Area:424513.5 TEH Amount: 12.99185

Batch ID: 163190

LCS-163190 ;0124HP5 ,

G:\org\HP5\DAT\HP5012422\_b\0124HP5.0056.RAW



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: LCS-163190 ;0124HP5 ,  
Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0056.RAW  
Date & Time Acquired: 1/25/2022 11:40:13 PM  
Method File: G:\Org\HP5\Methods\D3\_8015-C24-JC-L%.met  
Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111Jc-C24.CAL  
Sample Weight: 1000 Dilution: 1 S.A.: 1


Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.58 to 14.47

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.305	.2	.303	151.44	-
*1-Chlorooctadecane	13.155	.2	.184	92.08	-

DRO Area: 3.769579E+08 DRO Amount: 11.53646  
TEH Area: 4.029441E+08 TEH Amount: 12.33174





**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**


Sample Name: LCS-163190 ;0124HP5 ,  
 Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0056.RAW  
 Date & Time Acquired: 1/25/2022 11:40:13 PM  
 Method File: G:\Org\HP5\Methods\DS\_8015-C24-JC-L#.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JC-C24.CAL  
 Sample Weight: 1000 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.58 to 14.47

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	12.305	.2	.176	87.88
*1-Chlorooctadecane	13.155	.2	.051	25.37

DRO Area:1.750423E+08 DRO Amount: 5.357012  
 TEH Area:1.870454E+08 TEH Amount: 5.724355



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**


Sample Name: LCSD-163190 ;0124HP5 ,  
 Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0057.RAW  
 Date & Time Acquired: 1/26/2022 12:23:04 AM  
 Method File: G:\Org\HP5\Methods\D3\_8015-C24-JC-L%.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111Jc-C24.CAL  
 Sample Weight: 1000 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.58 to 14.47

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.307	.2	.305	152.51	-
*1-Chlorooctadecane	13.156	.2	.181	90.52	-

DRO Area: 3.725365E+08 DRO Amount: 11.40115  
 TEH Area: 3.987229E+08 TEH Amount: 12.20256



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**


Sample Name: LCSD-163190 ;0124HP5 ,  
 Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0057.RAW  
 Date & Time Acquired: 1/26/2022 12:23:04 AM  
 Method File: G:\Org\HP5\Methods\DS\_8015-C24-JC-L#.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JC-C24.CAL  
 Sample Weight: 1000 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.58 to 14.47

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	12.307	.2	.176	88.03
*1-Chlorooctadecane	13.156	.2	.05	25.07

DRO Area: 1.745379E+08 DRO Amount: 5.341577  
 TEH Area: 1.866121E+08 TEH Amount: 5.711095



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: MB-163190 ;0124HP5 ,  
 Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0058.RAW  
 Date & Time Acquired: 1/26/2022 1:05:50 AM  
 Method File: G:\Org\HP5\Methods\DR\_8015-C24T-JC-L%.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JC-C24-T.CAL  
 Sample Weight: 1000 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36


Rt range for Diesel Range Organics: 6.58 to 14.47

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.304	.2	.191	95.6	-
*1-Chlorooctadecane	13.146	.2	.	.05	-
*#Triacontane	16.389	.2	.097	48.47	-

DRO Area:351469.1 DRO Amount: 0.0107564  
 TEH Area:595369 TEH Amount: 1.822073E-02

G:\org\HP5\DAT\HP5012422\_b\0124HP5.0058.RAW

MB-163190 ;0124HP5 ,




**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: MB-163190 ;0124HP5 ,  
Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0058.RAW  
Date & Time Acquired: 1/26/2022 1:05:50 AM  
Method File: G:\Org\HP5\Methods\DR\_OROS-BC-L%.MET  
Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BC\_SAMP.CAL  
Sample Weight: 1000 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 26424.55  
Rt range for Residual Range Organics: 14.37 to 21.94

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*#Triacontane_____	16.389	.5	.097	19.39

RRO Area:169763.5 RRO AMOUNT: 6.42446E-03



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: MB-163190 ;0124HP5 ,  
Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0058.RAW  
Date & Time Acquired: 1/26/2022 1:05:50 AM  
Method File: G:\Org\HP5\Methods\DS\_8015-C24T-JC-L#.met  
Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JC-C24-T.CAL  
Sample Weight: 1000 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.58 to 14.47

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	12.304	.2	.19	95.17
*1-Chlorooctadecane	29.988	.2	.	-
*#Triacontane	16.389	.2	.096	47.96


DRO Area:174840.3 DRO Amount: 5.35083E-03  
TEH Area:574130.4 TEH Amount: 1.757074E-02

ERH2456 (RHMW13 zone 5)

Batch ID: 163190

G:\org\HP5\DAT\HP5012422\_b\0124HP5.0059.RAW

B22011446-006D ;0124HP5 , \$HC-8015-DRO-W,



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: B22011446-006D ;0124HP5 , \$HC-8015-DRO-W,  
Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0059.RAW  
Date & Time Acquired: 1/26/2022 1:48:36 AM  
Method File: G:\Org\HP5\Methods\DR\_8015-C24T-JC-L%.met  
Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JC-C24-T.CAL  
Sample Weight: 990 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.58 to 14.47

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.303	.202	.182	90.34	-
*1-Chlorooctadecane	13.126	.202	.	.05	-
*#Triacontane	16.388	.202	.093	46.04	-


DRO Area:952732.2 DRO Amount: 2.945203E-02  
TEH Area:1228798 TEH Amount: 0.0379861

ERH2456 (RHMW13 zone 5)

Batch ID: 163190

G:\org\HP5\DAT\HP5012422\_b\0124HP5.0059.RAW

B22011446-006D ;0124HP5 , \$HC-8015-DRO-W,



**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: B22011446-006D ;0124HP5 , \$HC-8015-DRO-W,  
Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0059.RAW  
Date & Time Acquired: 1/26/2022 1:48:36 AM  
Method File: G:\Org\HP5\Methods\DR\_OROS-BC-L%.MET  
Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BC\_SAMP.CAL  
Sample Weight: 990 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 26424.55  
Rt range for Residual Range Organics: 14.37 to 21.94

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*#Triacontane_____	16.388	.505	.093	18.42

RRO Area:217830.5 RRO AMOUNT: 8.326758E-03




ERH2456 (RHMW13 zone 5)

Batch ID: 163190

G:\org\HP5\DAT\HP5012422\_b\0124HP5.0059.RAW

B22011446-006D ;0124HP5 , \$HC-8015-DRO-W,



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: B22011446-006D ;0124HP5 , \$HC-8015-DRO-W,  
Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0059.RAW  
Date & Time Acquired: 1/26/2022 1:48:36 AM  
Method File: G:\Org\HP5\Methods\DS\_8015-C24T-JC-L#.met  
Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JC-C24-T.CAL  
Sample Weight: 990 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.58 to 14.47

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.303	.202	.181	89.82	-
*1-Chlorooctadecane	13.166	.202	.	.02	-
*#Triacontane	16.388	.202	.092	45.61	-


DRO Area:547866.1 DRO Amount: 1.693631E-02  
TEH Area:932518.3 TEH Amount: 2.882716E-02

ERH2439 (RHMW2254-01 LF)

Batch ID: 163190

G:\org\HP5\DAT\HP5012422\_b\0124HP5.0060.RAW

B22011446-017D ;0124HP5 , \$HC-8015-DRO-W,



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: B22011446-017D ;0124HP5 , \$HC-8015-DRO-W,  
Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0060.RAW  
Date & Time Acquired: 1/26/2022 2:31:22 AM  
Method File: G:\Org\HP5\Methods\D3\_8015-012460-JC-L%.met  
Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JC-C24-T.CAL  
Sample Weight: 1030 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.58 to 14.47

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.302	.194	.18	92.82	-
*1-Chlorooctadecane	13.149	.194	.005	2.77	-
*#Triacontane	16.388	.194	.117	60.23	-

DRO Area:1.988011E+07 DRO Amount: 0.5906921


TEH Area:3.399236E+07 TEH Amount: 1.010005

ERH2439 (RHMW2254-01 LF)

Batch ID: 163190

G:\org\HP5\DAT\HP5012422\_b\0124HP5.0060.RAW

B22011446-017D ;0124HP5 , \$HC-8015-DRO-W,



**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: B22011446-017D ;0124HP5 , \$HC-8015-DRO-W,  
Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0060.RAW  
Date & Time Acquired: 1/26/2022 2:31:22 AM  
Method File: G:\Org\HP5\Methods\D3\_OROS-BC-L%.MET  
Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BC\_SAMP.CAL  
Sample Weight: 1030 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 26424.55  
Rt range for Residual Range Organics: 14.37 to 21.94

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*#Triacontane_____	16.388	.485	.117	24.19


RRO Area:1.205952E+07 RRO AMOUNT: 0.4430831

ERH2439 (RHMW2254-01 LF)

Batch ID: 163190

G:\org\HP5\DAT\HP5012422\_b\0124HP5.0060.RAW

B22011446-017D ;0124HP5 , \$HC-8015-DRO-W,



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: B22011446-017D ;0124HP5 , \$HC-8015-DRO-W,  
Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0060.RAW  
Date & Time Acquired: 1/26/2022 2:31:22 AM  
Method File: G:\Org\HP5\Methods\DS\_8015-C24T-JC-L#.met  
Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JC-C24-T.CAL  
Sample Weight: 1030 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.58 to 14.47

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.302	.194	.172	88.83	-
*1-Chlorooctadecane	13.149	.194	.	.05	-
*#Triacontane	16.388	.194	.091	47.1	-

DRO Area:1.051956E+07 DRO Amount: 0.3125647


TEH Area:1.231335E+07 TEH Amount: 0.365863

ERH2452 (OWDFM07A)

Batch ID: 163190

G:\org\HP5\DAT\HP5012422\_b\0124HP5.0061.RAW

B22011446-027D ;0124HP5 , \$HC-8015-DRO-W,



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**


Sample Name: B22011446-027D ;0124HP5 , \$HC-8015-DRO-W,  
Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0061.RAW  
Date & Time Acquired: 1/26/2022 3:14:15 AM  
Method File: G:\Org\HP5\Methods\DR\_8015-C24T-JC-L0.met  
Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JC-C24-T.CAL  
Sample Weight: 1040 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.58 to 14.47

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.302	.192	.168	87.22	-
*1-Chlorooctadecane	13.157	.192	.	.17	-
*#Triacontane	16.388	.192	.088	45.69	-

DRO Area:1244546 DRO Amount: 3.662329E-02  
TEH Area:1602943 TEH Amount: 4.716984E-02



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: DCM-Baseline Check-V62  
 Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0062.RAW  
 Date & Time Acquired: 1/26/2022 3:57:00 AM  
 Method File: G:\Org\HP5\Methods\DR\_8015-JA-LEXP.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JA.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.63 to 15.99

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	29.925	200.	.	-
*1-Chlorooctadecane	29.925	200.	.	-


DRO Area:234099.8 DRO Amount: 7.164413  
 TEH Area:364603.8 TEH Amount: 11.15837

ERH2442 (Sump Adit3)

G:\org\HP5\DAT\HP5012422\_b\0124HP5.0063.RAW

Batch ID: 163190

B22011446-022D ;0124HP5 , \$HC-8015-DRO-W,



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: B22011446-022D ;0124HP5 , \$HC-8015-DRO-W,  
Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0063.RAW  
Date & Time Acquired: 1/26/2022 4:39:52 AM  
Method File: G:\Org\HP5\Methods\D3\_8015-C24T-JC-L%.met  
Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JC-C24-T.CAL  
Sample Weight: 1020 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.58 to 14.47

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.301	.196	.179	91.48	-
*1-Chlorooctadecane	13.156	.196	.004	1.96	-
*#Triacontane	16.385	.196	.102	52.22	-


DRO Area: 3.468403E+07 DRO Amount: 1.04066  
TEH Area: 4.742224E+07 TEH Amount: 1.422858

ERH2442 (Sump Adit3)

Batch ID: 163190

G:\org\HP5\DAT\HP5012422\_b\0124HP5.0063.RAW

B22011446-022D ;0124HP5 , \$HC-8015-DRO-W,



**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: B22011446-022D ;0124HP5 , \$HC-8015-DRO-W,  
Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0063.RAW  
Date & Time Acquired: 1/26/2022 4:39:52 AM  
Method File: G:\Org\HP5\Methods\D3\_OROS-BC-L%.MET  
Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BC\_SAMP.CAL  
Sample Weight: 1020 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 26424.55  
Rt range for Residual Range Organics: 14.37 to 21.94

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*#Triacontane_____	16.385	.49	.102	20.88

RRO Area:1.03215E+07 RRO AMOUNT: 0.3829437




ERH2442 (Sump Adit3)

Batch ID: 163190

G:\org\HP5\DAT\HP5012422\_b\0124HP5.0063.RAW

B22011446-022D ;0124HP5 , \$HC-8015-DRO-W,



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: B22011446-022D ;0124HP5 , \$HC-8015-DRO-W,  
Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0063.RAW  
Date & Time Acquired: 1/26/2022 4:39:52 AM  
Method File: G:\Org\HP5\Methods\DS\_8015-C24T-JC-L#.met  
Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JC-C24-T.CAL  
Sample Weight: 1020 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.58 to 14.47

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.301	.196	.171	87.45	-
*1-Chlorooctadecane	13.156	.196	.	.12	-
*#Triacontane	16.385	.196	.088	44.63	-

DRO Area: 1.902817E+07 DRO Amount: 0.5709217


TEH Area: 2.016237E+07 TEH Amount: 0.6049523

ERH2437 (RHMW2254-01 Bailer)

Batch ID: 163190

G:\org\HP5\DAT\HP5012422\_b\0124HP5.0064.RAW

B22011446-012B ;0124HP5 , \$HC-8015-DRO-W,



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: B22011446-012B ;0124HP5 , \$HC-8015-DRO-W,  
Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0064.RAW  
Date & Time Acquired: 1/26/2022 5:22:34 AM  
Method File: G:\Org\HP5\Methods\D3\_8015-C24T-JC-L%.met  
Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JC-C24-T.CAL  
Sample Weight: 1030 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.58 to 14.47

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.301	.194	.18	92.7	-
*1-Chlorooctadecane	29.791	.194	.	.	-
*#Triacontane	16.383	.194	.114	58.82	-

DRO Area:1.255819E+07 DRO Amount: 0.3731379


TEH Area:2.358476E+07 TEH Amount: 0.7007675

ERH2437 (RHMW2254-01 Bailer)

Batch ID: 163190

G:\org\HP5\DAT\HP5012422\_b\0124HP5.0064.RAW

B22011446-012B ;0124HP5 , \$HC-8015-DRO-W,



**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: B22011446-012B ;0124HP5 , \$HC-8015-DRO-W,  
Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0064.RAW  
Date & Time Acquired: 1/26/2022 5:22:34 AM  
Method File: G:\Org\HP5\Methods\D3\_OROS-BC-L%.MET  
Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BC\_SAMP.CAL  
Sample Weight: 1030 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 26424.55  
Rt range for Residual Range Organics: 14.37 to 21.94

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*#Triacontane_____	16.383	.485	.114	23.53


RRO Area:9122947 RRO AMOUNT: 0.3351894

ERH2437 (RHMW2254-01 Bailer)

Batch ID: 163190

G:\org\HP5\DAT\HP5012422\_b\0124HP5.0064.RAW

B22011446-012B ;0124HP5 , \$HC-8015-DRO-W,



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: B22011446-012B ;0124HP5 , \$HC-8015-DRO-W,  
Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0064.RAW  
Date & Time Acquired: 1/26/2022 5:22:34 AM  
Method File: G:\Org\HP5\Methods\DS\_8015-C24T-JC-L#.met  
Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JC-C24-T.CAL  
Sample Weight: 1030 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.58 to 14.47

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	12.301	.194	.172	88.82
*1-Chlorooctadecane	29.93	.194	.	-
*#Triacontane	16.383	.194	.094	48.63


DRO Area:2517506 DRO Amount: 7.480194E-02  
TEH Area:2877514 TEH Amount: 8.549876E-02

ERH2435 (RHMW2254-01 Bailer)

Batch ID: 163190

G:\org\HP5\DAT\HP5012422\_b\0124HP5.0065.RAW

B22011446-011D ;0124HP5 , \$HC-8015-DRO-W,



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: B22011446-011D ;0124HP5 , \$HC-8015-DRO-W,  
Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0065.RAW  
Date & Time Acquired: 1/26/2022 6:05:20 AM  
Method File: G:\Org\HP5\Methods\D3\_8015-C24T-JC-L%.met  
Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JC-C24-T.CAL  
Sample Weight: 1010 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.58 to 14.47

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.299	.198	.127	63.88	-
*1-Chlorooctadecane	29.715	.198	.	.	-
*#Triacontane	16.382	.198	.105	52.79	-

DRO Area:1.028414E+07 DRO Amount: 0.3116207


TEH Area:1.915033E+07 TEH Amount: 0.580276

ERH2435 (RHMW2254-01 Bailer)

Batch ID: 163190

G:\org\HP5\DAT\HP5012422\_b\0124HP5.0065.RAW

B22011446-011D ;0124HP5 , \$HC-8015-DRO-W,



**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: B22011446-011D ;0124HP5 , \$HC-8015-DRO-W,  
Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0065.RAW  
Date & Time Acquired: 1/26/2022 6:05:20 AM  
Method File: G:\Org\HP5\Methods\D3\_OROS-BC-L%.MET  
Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BC\_SAMP.CAL  
Sample Weight: 1010 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 26424.55  
Rt range for Residual Range Organics: 14.37 to 21.94

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*#Triacontane_____	16.382	.495	.105	21.12


RRO Area:6324467 RRO AMOUNT: 0.2369708

ERH2435 (RHMW2254-01 Bailer)

Batch ID: 163190

G:\org\HP5\DAT\HP5012422\_b\0124HP5.0065.RAW

B22011446-011D ;0124HP5 , \$HC-8015-DRO-W,



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**


Sample Name: B22011446-011D ;0124HP5 , \$HC-8015-DRO-W,  
Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0065.RAW  
Date & Time Acquired: 1/26/2022 6:05:20 AM  
Method File: G:\Org\HP5\Methods\DS\_8015-C24T-JC-L#.met  
Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JC-C24-T.CAL  
Sample Weight: 1010 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.58 to 14.47

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	12.299	.198	.12	60.82
*1-Chlorooctadecane	29.715	.198	.	-
*#Triacontane	16.382	.198	.092	46.68

DRO Area:2301609 DRO Amount: 6.974126E-02  
TEH Area:3417269 TEH Amount: 0.103547



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: DCM-Baseline Check-V66  
 Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0066.RAW  
 Date & Time Acquired: 1/26/2022 6:48:10 AM  
 Method File: G:\Org\HP5\Methods\DR\_8015-JA-LEXP.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JA.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36  
 Rt range for Diesel Range Organics: 6.63 to 15.99

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	28.58	200.	.	-
*1-Chlorooctadecane	28.58	200.	.	-

DRO Area:297921.1 DRO Amount: 9.117607  
 TEH Area:888483.5 TEH Amount: 27.19124




ERH2462 (RHMW11-05)

Batch ID: 163190

G:\org\HP5\DAT\HP5012422\_b\0124HP5.0067.RAW

B22011446-032D ;0124HP5 , \$HC-8015-DRO-W,



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: B22011446-032D ;0124HP5 , \$HC-8015-DRO-W,  
Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0067.RAW  
Date & Time Acquired: 1/26/2022 7:30:56 AM  
Method File: G:\Org\HP5\Methods\DR\_8015-C24T-JC-L%.met  
Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JC-C24-T.CAL  
Sample Weight: 990 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.58 to 14.47

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.303	.202	.173	85.4	-
*1-Chlorooctadecane	13.167	.202	.001	.4	-
*#Triacontane	16.389	.202	.089	44.	-


DRO Area:829487.9 DRO Amount: 2.564215E-02  
TEH Area:1170675 TEH Amount: 3.618934E-02

ERH2462 (RHMW11-05)

Batch ID: 163190

G:\org\HP5\DAT\HP5012422\_b\0124HP5.0067.RAW

B22011446-032D ;0124HP5 , \$HC-8015-DRO-W,



**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: B22011446-032D ;0124HP5 , \$HC-8015-DRO-W,  
Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0067.RAW  
Date & Time Acquired: 1/26/2022 7:30:56 AM  
Method File: G:\Org\HP5\Methods\DR\_OROS-BC-L%.MET  
Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BC\_SAMP.CAL  
Sample Weight: 990 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 26424.55  
Rt range for Residual Range Organics: 14.37 to 21.94

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*#Triacontane_____	16.389	.505	.089	17.6


RRO Area:258295.7 RRO AMOUNT: 9.873572E-03

ERH2462 (RHMW11-05)

Batch ID: 163190

G:\org\HP5\DAT\HP5012422\_b\0124HP5.0067.RAW

B22011446-032D ;0124HP5 , \$HC-8015-DRO-W,




**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**


Sample Name: B22011446-032D ;0124HP5 , \$HC-8015-DRO-W,  
Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0067.RAW  
Date & Time Acquired: 1/26/2022 7:30:56 AM  
Method File: G:\Org\HP5\Methods\DS\_8015-C24T-JC-L#.met  
Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JC-C24-T.CAL  
Sample Weight: 990 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36  
Rt range for Diesel Range Organics: 6.58 to 14.47

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.303	.202	.171	84.74	-
*1-Chlorooctadecane	13.167	.202	.001	.31	-
*#Triacontane	16.389	.202	.088	43.6	-

DRO Area:543192.4 DRO Amount: 1.679184E-02  
TEH Area:981653.2 TEH Amount: 3.034607E-02





**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: CCV\_0124HP569r, RRO ;0124HP5 , DRO220118A  
 Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0069.RAW  
 Date & Time Acquired: 1/26/2022 8:56:23 AM  
 Method File: G:\Org\HP5\Methods\DC\_ORO-BC-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BC.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for for ~~Residual~~ TEH(Oil Range) Organics Calculations: 26424.55  
 Rt range for ~~Residual~~ TEH(Oil Range) Organics: 12.65 to 30.05

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*#Triacontane	16.389	500.	325.308	65.06	-

RRO TEH(Oil Range) Area: 1.203064E+08 RRO TEH(Oil Range) AMOUNT: 4552.825


CONTINUING CALIBRATION REPORT: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0069.RAW

COMPOUND	ACTUAL (NG)	MEASURED (NG)	%RECOVERY	LIMITS
*30-40 Motor Oil	5000.	.05	.	75-125

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	LIMITS
*#Triacontane	16.389	200.	325.308	162.65	75-125

AMN 02/15/2022



**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: CCV\_0124HP569r, RRO ;0124HP5 , DRO220118A  
 Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0069.RAW  
 Date & Time Acquired: 1/26/2022 8:56:23 AM  
 Method File: G:\Org\HP5\Methods\DS\_ORO-BC-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BC.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 26424.55  
 Rt range for Residual Range Organics: 12.65 to 30.05

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*#Triacontane	16.389	500.	204.488	40.9


RRO Area:3131369 RRO AMOUNT: 118.5022

**CONTINUING CALIBRATION REPORT: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0069.RAW**

COMPOUND	ACTUAL (NG)	MEASURED (NG)	%RECOVERY	LIMITS
*30-40 Motor Oil	5000.	.05	.	75-125

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	LIMITS
*#Triacontane	16.389	200.	204.488	102.24	75-125



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: CCV\_0124HP570r, DRO ;0124HP5 , DRO220124A  
 Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0070.RAW  
 Date & Time Acquired: 1/26/2022 9:39:21 AM  
 Method File: G:\Org\HP5\Methods\DC\_8015-C24-JC-L%.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JC-C24.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36  
 Rt range for Diesel Range Organics: 6.58 to 14.47

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	12.302	200.	293.15	146.58
*1-Chlorooctadecane	13.149	200.	138.455	69.23

DRO Area: 4.247823E+08 DRO Amount: 13000.08  
 TEH Area: 4.395158E+08 TEH Amount: 13450.99


CONTINUING CALIBRATION REPORT: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0070.RAW

COMPOUND	ACTUAL (NG)	MEASURED (NG)	%RECOVERY	LIMITS
TOTAL DRO	15000.	13450.99	89.67	85-115

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	LIMITS
*o-Terphenyl	12.302	200.	293.15	146.58	85-115
*1-Chlorooctadecane	13.149	200.	138.455	69.23	85-115

G:\org\HP5\DAT\HP5012422\_b\0124HP5.0070.RAW

CCV\_0124HP570r, DRO ;0124HP5 , DRO220124A



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: CCV\_0124HP570r, DRO ;0124HP5 , DRO220124A  
 Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0070.RAW  
 Date & Time Acquired: 1/26/2022 9:39:21 AM  
 Method File: G:\Org\HP5\Methods\DS\_8015-C24-JC-L#.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JC-C24.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.58 to 14.47

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	12.302	200.	178.601	89.3
*1-Chlorooctadecane	13.149	200.	32.377	16.19


DRO Area: 2.189839E+08 DRO Amount: 6701.805  
 TEH Area: 2.284265E+08 TEH Amount: 6990.789

CONTINUING CALIBRATION REPORT: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0070.RAW

COMPOUND	ACTUAL (NG)	MEASURED (NG)	%RECOVERY	LIMITS
TOTAL DRO	15000.	6990.79	46.61	85-115

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	LIMITS
*o-Terphenyl	12.302	200.	178.601	89.3	85-115
*1-Chlorooctadecane	13.149	200.	32.377	16.19	85-115






**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: DCM-Baseline Check-V71  
 Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0071.RAW  
 Date & Time Acquired: 1/26/2022 10:22:28 AM  
 Method File: G:\Org\HP5\Methods\DR\_8015-JA-LEXP.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JA.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36  
 Rt range for Diesel Range Organics: 6.63 to 15.99

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	29.465	200.	.	-
*1-Chlorooctadecane	13.18	200.	.018	.01 -

DRO Area:307888 DRO Amount: 9.422635  
 TEH Area:599350.4 TEH Amount: 18.34258



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: DCM-Baseline Check-V72  
 Raw File: G:\Org\HP5\DAT\HP5012422\_b\0124HP5.0072.RAW  
 Date & Time Acquired: 1/26/2022 11:05:17 AM  
 Method File: G:\Org\HP5\Methods\DR\_8015-JA-LEXP.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JA.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.63 to 15.99

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.377	200.	.018	.01	-
*1-Chlorooctadecane	13.196	200.	.026	.01	-


DRO Area:263182.4 DRO Amount: 8.05446  
 TEH Area:446345.1 TEH Amount: 13.65999

ERH2470 (RHMW19)

Batch ID: 163190

G:\org\HP5\DAT\HP5012422\_b\0124HP5.0073.RAW

B22011446-001D ;0124HP5 , \$HC-8015-DRO-W,



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: B22011446-001D ;0124HP5 , \$HC-8015-DRO-W,  
Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0073.RAW  
Date & Time Acquired: 1/26/2022 11:48:03 AM  
Method File: G:\Org\HP5\Methods\D3\_8015-C24T-JC-L%.met  
Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JC-C24-T.CAL  
Sample Weight: 1010 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.58 to 14.47

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.301	.198	.169	85.27	-
*1-Chlorooctadecane	13.155	.198	.001	.32	-
*#Triacontane	16.387	.198	.096	48.57	-


DRO Area:1572873 DRO Amount: 4.765976E-02  
TEH Area:7467341 TEH Amount: 0.2262686

ERH2470 (RHMW19)

Batch ID: 163190

G:\org\HP5\DAT\HP5012422\_b\0124HP5.0073.RAW

B22011446-001D ;0124HP5 , \$HC-8015-DRO-W,



**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: B22011446-001D ;0124HP5 , \$HC-8015-DRO-W,  
Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0073.RAW  
Date & Time Acquired: 1/26/2022 11:48:03 AM  
Method File: G:\Org\HP5\Methods\D3\_OROS-BC-L%.MET  
Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BC\_SAMP.CAL  
Sample Weight: 1010 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 26424.55  
Rt range for Residual Range Organics: 14.37 to 21.94

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*#Triacontane_____	16.387	.495	.096	19.43


RRO Area:4490057 RRO AMOUNT: 0.1682375

ERH2470 (RHMW19)

Batch ID: 163190

G:\org\HP5\DAT\HP5012422\_b\0124HP5.0073.RAW

B22011446-001D ;0124HP5 , \$HC-8015-DRO-W,



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: B22011446-001D ;0124HP5 , \$HC-8015-DRO-W,  
 Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0073.RAW  
 Date & Time Acquired: 1/26/2022 11:48:03 AM  
 Method File: G:\Org\HP5\Methods\DS\_8015-C24T-JC-L#.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JC-C24-T.CAL  
 Sample Weight: 1010 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.58 to 14.47

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.301	.198	.166	83.61	-
*1-Chlorooctadecane	13.155	.198	.	.01	-
*#Triacontane	16.387	.198	.086	43.64	-


DRO Area:641124.1 DRO Amount: 1.942676E-02  
 TEH Area:998085.7 TEH Amount: 3.024308E-02

ERH2452 (OWDFMW07A)

Batch ID: 163190

G:\org\HP5\DAT\HP5012422\_b\0124HP5.0074.RAW

B22011446-027D ;0124HP5 , \$HC-8015-DRO-W, RR



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: B22011446-027D ;0124HP5 , \$HC-8015-DRO-W, RR  
 Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0074.RAW  
 Date & Time Acquired: 1/26/2022 12:30:49 PM  
 Method File: G:\Org\HP5\Methods\DR\_8015-C24T-JC-L%.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JC-C24-T.CAL  
 Sample Weight: 1040 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.58 to 14.47

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.301	.192	.173	89.99	-
*1-Chlorooctadecane	13.16	.192	.	.09	-
*#Triacontane	16.387	.192	.087	45.4	-


DRO Area: 685602.8 DRO Amount: 2.017525E-02  
 TEH Area: 953293.1 TEH Amount: 2.805257E-02

ERH2452 (OWDFMW07A)

Batch ID: 163190

G:\org\HP5\DAT\HP5012422\_b\0124HP5.0074.RAW

B22011446-027D ;0124HP5 , \$HC-8015-DRO-W, RR



**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: B22011446-027D ;0124HP5 , \$HC-8015-DRO-W, RR  
 Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0074.RAW  
 Date & Time Acquired: 1/26/2022 12:30:49 PM  
 Method File: G:\Org\HP5\Methods\DR\_OROS-BC-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BC\_SAMP.CAL  
 Sample Weight: 1040 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 26424.55  
 Rt range for Residual Range Organics: 14.37 to 21.94

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*#Triacontane_____	16.387	.481	.087	18.16


RRO Area:185335 RRO AMOUNT: 6.743983E-03

ERH2452 (OWDFM07A)

Batch ID: 163190

G:\org\HP5\DAT\HP5012422\_b\0124HP5.0074.RAW

B22011446-027D ;0124HP5 , \$HC-8015-DRO-W, RR



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: B22011446-027D ;0124HP5 , \$HC-8015-DRO-W, RR  
 Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0074.RAW  
 Date & Time Acquired: 1/26/2022 12:30:49 PM  
 Method File: G:\Org\HP5\Methods\DS\_8015-C24T-JC-L#.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JC-C24-T.CAL  
 Sample Weight: 1040 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.58 to 14.47

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.301	.192	.172	89.38	-
*1-Chlorooctadecane	13.16	.192	.	.01	-
*Triacontane	16.387	.192	.086	44.76	-

DRO Area:400981.9  
 TEH Area:751581.6


DRO Amount: 0.0117997  
 TEH Amount: 2.211681E-02



Batch ID: 163190

B22011446-001DMS ;0124HP5 ,

G:\org\HP5\DAT\HP5012422\_b\0124HP5.0075.RAW



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: B22011446-001DMS ;0124HP5 ,  
 Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0075.RAW  
 Date & Time Acquired: 1/26/2022 1:13:32 PM  
 Method File: G:\Org\HP5\Methods\D3\_8015-012475-JC-L%.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111Jc-C24.CAL  
 Sample Weight: 990 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.58 to 14.47


SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.304	.202	.331	164.	-
*1-Chlorooctadecane	13.151	.202	.152	75.42	-

DRO Area: 4.269073E+08 DRO Amount: 13.19709  
 TEH Area: 4.679144E+08 TEH Amount: 14.46475

Batch ID: 163190

G:\org\HP5\DAT\HP5012422\_b\0124HP5.0075.RAW

B22011446-001DMS ;0124HP5 ,



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**


Sample Name: B22011446-001DMS ;0124HP5 ,  
 Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0075.RAW  
 Date & Time Acquired: 1/26/2022 1:13:32 PM  
 Method File: G:\Org\HP5\Methods\DS\_8015-C24-JC-L#.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JC-C24.CAL  
 Sample Weight: 990 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.58 to 14.47

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	12.304	.202	.193	95.59
*1-Chlorooctadecane	13.151	.202	.056	27.78

DRO Area: 1.976423E+08 DRO Amount: 6.109762  
 TEH Area: 2.110373E+08 TEH Amount: 6.523845



**RESIDUAL RANGE ORGANICS CHROMATOGRAM**


Sample Name: B22011446-006DMS-RRO ;0124HP5 ,  
 Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0076.RAW  
 Date & Time Acquired: 1/26/2022 1:56:08 PM  
 Method File: G:\Org\HP5\Methods\D3\_ORO-BC-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111Bc.CAL  
 Sample Weight: 1060 Dilution: 1 S.A.: 1

Mean RF for for ~~Residual~~ TEH(Oil Range) Organics Calculations: 26424.55  
 Rt range for ~~Residual~~ TEH(Oil Range) Organics: 12.65 to 30.05

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*#Triacontane	16.386	.472	.174	36.8	-

~~RRO~~ TEH(Oil Range) Area:1.330668E+08 ~~RRO~~ TEH(Oil Range) AMOUNT: 4.750686

AMN 02/15/2022




**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: B22011446-006DMS-RRO ;0124HP5 ,  
 Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0076.RAW  
 Date & Time Acquired: 1/26/2022 1:56:08 PM  
 Method File: G:\Org\HP5\Methods\DS\_ORO-BC-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BC.CAL  
 Sample Weight: 1060 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 26424.55  
 Rt range for Residual Range Organics: 12.65 to 30.05

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*#Triacontane	16.386	.472	.09	18.99

RRO Area:2559530 RRO AMOUNT: 9.137907E-02



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**


Sample Name: DCM-Baseline Check-V77  
 Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0077.RAW  
 Date & Time Acquired: 1/26/2022 2:38:45 PM  
 Method File: G:\Org\HP5\Methods\DR\_8015-JA-LEXP.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JA.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.63 to 15.99

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.322	200.	12.008	6.	-
*1-Chlorooctadecane	13.137	200.	2.396	1.2	-

DRO Area: 7670507 DRO Amount: 234.749  
 TEH Area: 8649815 TEH Amount: 264.7198



**RESIDUAL RANGE ORGANICS CHROMATOGRAM**


Sample Name: LCS-163190-RRO ;0124HP5 ,  
 Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0078.RAW  
 Date & Time Acquired: 1/26/2022 3:21:18 PM  
 Method File: G:\Org\HP5\Methods\D3\_ORO-BC-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111Bc.CAL  
 Sample Weight: 1000 Dilution: 1 S.A.: 1

Mean RF for for ~~Residual~~ TEH(Oil Range) Organics Calculations: 26424.55  
 Rt range for ~~Residual~~ TEH(Oil Range) Organics: 12.65 to 30.05

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*#Triacontane_____	16.387	.5	.198	39.55 -

RRO TEH(Oil Range) Area:1.325448E+08 RRO TEH(Oil Range) AMOUNT: 5.015971

AMN 02/15/2022




**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: LCS-163190-RRO ;0124HP5 ,  
 Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0078.RAW  
 Date & Time Acquired: 1/26/2022 3:21:18 PM  
 Method File: G:\Org\HP5\Methods\DS\_ORO-BC-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BC.CAL  
 Sample Weight: 1000 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 26424.55  
 Rt range for Residual Range Organics: 12.65 to 30.05

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*#Triacontane	16.387	.5	.096	19.2

RRO Area:2941369 RRO AMOUNT: 0.111312



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**


Sample Name: DCM-Baseline Check-V79  
 Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0079.RAW  
 Date & Time Acquired: 1/26/2022 4:03:53 PM  
 Method File: G:\Org\HP5\Methods\DR\_8015-JA-LEXP.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JA.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36  
 Rt range for Diesel Range Organics: 6.63 to 15.99

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	29.976	200.	.	.
*1-Chlorooctadecane	29.976	200.	.	.

DRO Area:172944.6 DRO Amount: 5.292814  
 TEH Area:781432.8 TEH Amount: 23.91505





**RESIDUAL RANGE ORGANICS CHROMATOGRAM**


Sample Name: LCSD-163190-RRO ;0124HP5 ,  
 Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0080.RAW  
 Date & Time Acquired: 1/26/2022 4:46:20 PM  
 Method File: G:\Org\HP5\Methods\D3\_ORO-BC-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111Bc.CAL  
 Sample Weight: 1000 Dilution: 1 S.A.: 1

Mean RF for for ~~Residual~~ TEH(Oil Range) Organics Calculations: 26424.55  
 Rt range for ~~Residual~~ TEH(Oil Range) Organics: 12.65 to 30.05

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*#Triacontane	16.385	.5	.182	36.42	-

RRO TEH(Oil Range) Area:1.304655E+08 RRO TEH(Oil Range) AMOUNT: 4.937282

AMN 02/15/2022




**RESIDUAL RANGE ORGANICS CHROMATOGRAM**


Sample Name: LCSD-163190-RRO ;0124HP5 ,  
Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0080.RAW  
Date & Time Acquired: 1/26/2022 4:46:20 PM  
Method File: G:\Org\HP5\Methods\DS\_ORO-BC-L%.MET  
Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BC.CAL  
Sample Weight: 1000 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 26424.55  
Rt range for Residual Range Organics: 12.65 to 30.05

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*#Triacontane_____	16.385	.5	.093	18.66 -

RRO Area:2778595 RRO AMOUNT: 0.105152





**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: CCV\_0124HP583r, RRO ;0124HP5 , DRO220118A  
 Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0082.RAW  
 Date & Time Acquired: 1/26/2022 6:12:44 PM  
 Method File: G:\Org\HP5\Methods\DC\_ORO-BC-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BC.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for for ~~Residual~~ TEH(Oil Range) Organics Calculations: 26424.55  
 Rt range for ~~Residual~~ TEH(Oil Range) Organics: 12.65 to 30.05

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*#Triacontane	16.386	500.	328.862	65.77	-

~~RRO~~ TEH(Oil Range) Area:1.223377E+08 ~~RRO~~ TEH(Oil Range) AMOUNT: 4629.698


CONTINUING CALIBRATION REPORT: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0082.RAW

COMPOUND	ACTUAL (NG)	MEASURED (NG)	%RECOVERY	LIMITS
*30-40 Motor Oil	5000.	.046	.	75-125

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	LIMITS
*#Triacontane	16.386	200.	328.862	164.43	75-125

AMN 02/15/2022



**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: CCV\_0124HP583r, RRO ;0124HP5 , DRO220118A  
 Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0082.RAW  
 Date & Time Acquired: 1/26/2022 6:12:44 PM  
 Method File: G:\Org\HP5\Methods\DS\_ORO-BC-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BC.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 26424.55  
 Rt range for Residual Range Organics: 12.65 to 30.05

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*#Triacontane	16.386	500.	202.574	40.51


RRO Area:2693176 RRO AMOUNT: 101.9194

CONTINUING CALIBRATION REPORT: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0082.RAW

COMPOUND	ACTUAL (NG)	MEASURED (NG)	%RECOVERY	LIMITS
*30-40 Motor Oil	5000.	.046	.	75-125

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	LIMITS
*#Triacontane	16.386	200.	202.574	101.29	75-125



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: CCV\_0124HP584r, DRO ;0124HP5 , DRO220124A  
 Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0083.RAW  
 Date & Time Acquired: 1/26/2022 6:55:49 PM  
 Method File: G:\Org\HP5\Methods\DC\_8015-C24-JC-L%.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JC-C24.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36  
 Rt range for Diesel Range Organics: 6.58 to 14.47

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	12.306	200.	303.549	151.77
*1-Chlorooctadecane	13.15	200.	146.153	73.08

DRO Area: 4.419185E+08 DRO Amount: 13524.52  
 TEH Area: 4.562785E+08 TEH Amount: 13963.99


CONTINUING CALIBRATION REPORT: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0083.RAW

COMPOUND	ACTUAL (NG)	MEASURED (NG)	%RECOVERY	LIMITS
TOTAL DRO	15000.	13963.99	93.09	85-115

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	LIMITS
*o-Terphenyl	12.306	200.	303.549	151.77	85-115
*1-Chlorooctadecane	13.15	200.	146.153	73.08	85-115

G:\org\HP5\DAT\HP5012422\_b\0124HP5.0083.RAW

CCV\_0124HP584r, DRO ;0124HP5 , DRO220124A



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: CCV\_0124HP584r, DRO ;0124HP5 , DRO220124A  
 Raw File: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0083.RAW  
 Date & Time Acquired: 1/26/2022 6:55:49 PM  
 Method File: G:\Org\HP5\Methods\DS\_8015-C24-JC-L#.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JC-C24.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.58 to 14.47


SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	12.306	200.	186.045	93.02
*1-Chlorooctadecane	13.15	200.	32.947	16.47

DRO Area: 2.274391E+08 DRO Amount: 6960.569  
 TEH Area: 2.371515E+08 TEH Amount: 7257.809

CONTINUING CALIBRATION REPORT: G:\org\HP5\DAT\HP5012422\_b\0124HP5.0083.RAW

COMPOUND	ACTUAL (NG)	MEASURED (NG)	%RECOVERY	LIMITS
TOTAL DRO	15000.	7257.81	48.39	85-115

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	LIMITS
*o-Terphenyl	12.306	200.	186.045	93.02	85-115
*1-Chlorooctadecane	13.15	200.	32.947	16.47	85-115



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**


Sample Name: DCM-Baseline Check-V01  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0001.RAW  
 Date & Time Acquired: 1/27/2022 8:33:22 AM  
 Method File: G:\Org\HP5\Methods\DR\_8015-JA-LEXP.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JA.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36  
 Rt range for Diesel Range Organics: 6.63 to 15.99

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.354	200.	1.009	.5	-
*1-Chlorooctadecane	29.949	200.	.	.	-

DRO Area: 2678667 DRO Amount: 81.9782  
 TEH Area: 3455482 TEH Amount: 105.7519






**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**


Sample Name: DCM-Baseline Check-V02  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0002.RAW  
 Date & Time Acquired: 1/27/2022 9:15:50 AM  
 Method File: G:\Org\HP5\Methods\DR\_8015-JA-LEXP.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JA.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36  
 Rt range for Diesel Range Organics: 6.63 to 15.99

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.304	200.	.089	.04	-
*1-Chlorooctadecane	13.169	200.	.025	.01	-

DRO Area: 232799 DRO Amount: 7.124604  
 TEH Area: 301407.4 TEH Amount: 9.224301





**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: CCV\_0127HP504r, RRO ;0127HP5 , DRO220118A  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0004.RAW  
 Date & Time Acquired: 1/27/2022 10:41:27 AM  
 Method File: G:\Org\HP5\Methods\DC\_ORO-BD-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111Bd.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for for ~~Residual~~ TEH(Oil Range) Organics Calculations: 26424.55  
 Rt range for ~~Residual~~ TEH(Oil Range) Organics: 12.62 to 30.05

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*#Triacontane	16.358	500.	323.503	64.7	-

RRO TEH(Oil Range) Area:1.203413E+08 RRO TEH(Oil Range) AMOUNT: 4554.147


CONTINUING CALIBRATION REPORT: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0004.RAW

COMPOUND	ACTUAL (NG)	MEASURED (NG)	%RECOVERY	LIMITS
*30-40 Motor Oil	5000.	.032	.	75-125

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	LIMITS
*#Triacontane	16.358	200.	323.503	161.75	75-125

AMN 02/15/2022



**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: CCV\_0127HP504r, RRO ;0127HP5 , DRO220118A  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0004.RAW  
 Date & Time Acquired: 1/27/2022 10:41:27 AM  
 Method File: G:\Org\HP5\Methods\DS\_ORO-BD-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BD.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 26424.55  
 Rt range for Residual Range Organics: 12.62 to 30.05

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*#Triacontane	16.358	500.	205.274	41.05	-


RRO Area:2944795 RRO AMOUNT: 111.4416

**CONTINUING CALIBRATION REPORT: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0004.RAW**

COMPOUND	ACTUAL (NG)	MEASURED (NG)	%RECOVERY	LIMITS
*30-40 Motor Oil	5000.	.032	.	75-125

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	LIMITS
*#Triacontane	16.358	200.	205.274	102.64	75-125



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: CCV\_0127HP505r, DRO ;0127HP5 , DRO220124A  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0005.RAW  
 Date & Time Acquired: 1/27/2022 11:24:13 AM  
 Method File: G:\Org\HP5\Methods\DC\_8015-C24-JD-L%.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JD-C24.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.57 to 14.43

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	12.285	200.	299.276	149.64
*1-Chlorooctadecane	13.13	200.	142.062	71.03

DRO Area: 4.373249E+08 DRO Amount: 13383.94  
 TEH Area: 4.527986E+08 TEH Amount: 13857.49


CONTINUING CALIBRATION REPORT: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0005.RAW

COMPOUND	ACTUAL (NG)	MEASURED (NG)	%RECOVERY	LIMITS
TOTAL DRO	15000.	13857.49	92.38	85-115

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	LIMITS
*o-Terphenyl	12.285	200.	299.276	149.64	85-115
*1-Chlorooctadecane	13.13	200.	142.062	71.03	85-115

G:\org\HP5\DAT\HP5012722\_b\0127HP5.0005.RAW

CCV\_0127HP505r, DRO ;0127HP5 , DRO220124A



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: CCV\_0127HP505r, DRO ;0127HP5 , DRO220124A  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0005.RAW  
 Date & Time Acquired: 1/27/2022 11:24:13 AM  
 Method File: G:\Org\HP5\Methods\DS\_8015-C24-JD-L#.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JD-C24.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.57 to 14.43


SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	12.285	200.	184.095	92.05
*1-Chlorooctadecane	13.13	200.	33.51	16.75

DRO Area: 2.259827E+08 DRO Amount: 6915.997  
 TEH Area: 2.362003E+08 TEH Amount: 7228.697

CONTINUING CALIBRATION REPORT: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0005.RAW

COMPOUND	ACTUAL (NG)	MEASURED (NG)	%RECOVERY	LIMITS
TOTAL DRO	15000.	7228.7	48.19	85-115

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	LIMITS
*o-Terphenyl	12.285	200.	184.095	92.05	85-115
*1-Chlorooctadecane	13.13	200.	33.51	16.75	85-115



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: DCM-Baseline Check-V05  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0006.RAW  
 Date & Time Acquired: 1/27/2022 12:06:54 PM  
 Method File: G:\Org\HP5\Methods\DR\_8015-JA-LEXP.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JA.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1


Mean RF for TEH: 32675.36  
 Rt range for Diesel Range Organics: 6.63 to 15.99

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	29.964	200.	.	-
*1-Chlorooctadecane	29.964	200.	.	-

DRO Area:230552.8 DRO Amount: 7.05586  
 TEH Area:329705.6 TEH Amount: 10.09034

Batch ID: 163190  
LCS-163190 ;0127HP5 , SGT

G:\org\HP5\DAT\HP5012722\_b\0127HP5.0008.RAW



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: LCS-163190 ;0127HP5 , SGT  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0008.RAW  
 Date & Time Acquired: 1/27/2022 1:31:58 PM  
 Method File: G:\Org\HP5\Methods\D3\_8015-C24-JD-L%.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JD-C24.CAL  
 Sample Weight: 1000 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.57 to 14.43

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.281	.2	.299	149.34	-
*1-Chlorooctadecane	13.129	.2	.181	90.53	-


DRO Area: 3.61013E+08 DRO Amount: 11.04848  
 TEH Area: 3.839162E+08 TEH Amount: 11.74941



Batch ID: 163190

G:\org\HP5\DAT\HP5012722\_b\0127HP5.0008.RAW

LCS-163190 ;0127HP5 , SGT



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: LCS-163190 ;0127HP5 , SGT  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0008.RAW  
 Date & Time Acquired: 1/27/2022 1:31:58 PM  
 Method File: G:\Org\HP5\Methods\DS\_8015-C24-JD-L#.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JD-C24.CAL  
 Sample Weight: 1000 Dilution: 1 S.A.: 1


Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.57 to 14.43

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	12.281	.2	.177	88.29
*1-Chlorooctadecane	13.129	.2	.049	24.29

DRO Area:1.666477E+08 DRO Amount: 5.100103  
 TEH Area:1.763773E+08 TEH Amount: 5.397869

Batch ID: 163190  
LCSD-163190 ;0127HP5 , SGT



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: LCSD-163190 ;0127HP5 , SGT  
 Raw File: G:\Org\HP5\DAT\HP5012722\_b\0127HP5.0009.RAW  
 Date & Time Acquired: 1/27/2022 2:14:29 PM  
 Method File: G:\Org\HP5\Methods\D3\_8015-C24-JD-L%.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JD-C24.CAL  
 Sample Weight: 1000 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36  
 Rt range for Diesel Range Organics: 6.57 to 14.43


SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.283	.2	.305	152.3	-
*1-Chlorooctadecane	13.13	.2	.127	63.26	-

DRO Area: 3.557062E+08 DRO Amount: 10.88607  
 TEH Area: 3.771962E+08 TEH Amount: 11.54375

Batch ID: 163190

LCSD-163190 ;0127HP5 , SGT

G:\org\HP5\DAT\HP5012722\_b\0127HP5.0009.RAW



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**


Sample Name: LCSD-163190 ;0127HP5 , SGT  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0009.RAW  
 Date & Time Acquired: 1/27/2022 2:14:29 PM  
 Method File: G:\Org\HP5\Methods\DS\_8015-C24-JD-L#.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JD-C24.CAL  
 Sample Weight: 1000 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.57 to 14.43

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	12.283	.2	.18	90.01
*1-Chlorooctadecane	13.13	.2	.048	24.22

DRO Area: 1.606838E+08 DRO Amount: 4.917583  
 TEH Area: 1.693637E+08 TEH Amount: 5.183224



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: MB-163190 ;0127HP5 , SGT  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0010.RAW  
 Date & Time Acquired: 1/27/2022 2:56:52 PM  
 Method File: G:\Org\HP5\Methods\DR\_8015-C24T-JD-L%.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JD-C24-T.CAL  
 Sample Weight: 1000 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36


Rt range for Diesel Range Organics: 6.57 to 14.43

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.28	.2	.183	91.29	-
*1-Chlorooctadecane	13.136	.2	.04		-
*#Triacontane	16.352	.2	.088	44.09	-

DRO Area:278171.9 DRO Amount: 8.513201E-03  
 TEH Area:530249.6 TEH Amount: 1.622781E-02

G:\org\HP5\DAT\HP5012722\_b\0127HP5.0010.RAW

MB-163190 ;0127HP5 , SGT



**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: MB-163190 ;0127HP5 , SGT  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0010.RAW  
 Date & Time Acquired: 1/27/2022 2:56:52 PM  
 Method File: G:\Org\HP5\Methods\DR\_OROS-BD-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BD\_SAMP.CAL  
 Sample Weight: 1000 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 26424.55  
 Rt range for Residual Range Organics: 14.33 to 21.83


SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*#Triacontane_____	16.352	.5	.088	17.64

RRO Area:183146.5 RRO AMOUNT: 6.930921E-03

Batch ID: 163190

MB-163190 ;0127HP5 , SGT

G:\org\HP5\DAT\HP5012722\_b\0127HP5.0010.RAW



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: MB-163190 ;0127HP5 , SGT  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0010.RAW  
 Date & Time Acquired: 1/27/2022 2:56:52 PM  
 Method File: G:\Org\HP5\Methods\DS\_8015-C24T-JD-L#.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111Jd-C24-T.CAL  
 Sample Weight: 1000 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.57 to 14.43

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	12.28	.2	.182	91.15
*1-Chlorooctadecane	29.972	.2	.	-
*#Triacontane	16.352	.2	.088	43.88


DRO Area:169434.4 DRO Amount: 5.185387E-03  
 TEH Area:439928.8 TEH Amount: 1.346363E-02

ERH2456 (RHMW13 zone 5)

Batch ID: 163190

G:\org\HP5\DAT\HP5012722\_b\0127HP5.0011.RAW

B22011446-006D ;0127HP5 , \$HC-8015-DRO-W, SGT



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: B22011446-006D ;0127HP5 , \$HC-8015-DRO-W, SGT  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0011.RAW  
 Date & Time Acquired: 1/27/2022 3:39:18 PM  
 Method File: G:\Org\HP5\Methods\DR\_8015-C24T-JD-L%.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JD-C24-T.CAL  
 Sample Weight: 990 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.57 to 14.43

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.278	.202	.176	86.9	-
*1-Chlorooctadecane	13.132	.202	.	.03	-
*#Triacontane	16.354	.202	.088	43.51	-


DRO Area:294259.6 DRO Amount: 9.096516E-03  
 TEH Area:521507.3 TEH Amount: 1.612148E-02

ERH2456 (RHMW13 zone 5)

Batch ID: 163190

G:\org\HP5\DAT\HP5012722\_b\0127HP5.0011.RAW

B22011446-006D ;0127HP5 , \$HC-8015-DRO-W, SGT



**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: B22011446-006D ;0127HP5 , \$HC-8015-DRO-W, SGT  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0011.RAW  
 Date & Time Acquired: 1/27/2022 3:39:18 PM  
 Method File: G:\Org\HP5\Methods\DR\_OROS-BD-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BD\_SAMP.CAL  
 Sample Weight: 990 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 26424.55  
 Rt range for Residual Range Organics: 14.33 to 21.83

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*#Triacontane_____	16.354	.505	.088	17.4

RRO Area:178412.1 RRO AMOUNT: 6.819955E-03




ERH2456 (RHMW13 zone 5)

Batch ID: 163190

G:\org\HP5\DAT\HP5012722\_b\0127HP5.0011.RAW

B22011446-006D ;0127HP5 , \$HC-8015-DRO-W, SGT



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: B22011446-006D ;0127HP5 , \$HC-8015-DRO-W, SGT  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0011.RAW  
 Date & Time Acquired: 1/27/2022 3:39:18 PM  
 Method File: G:\Org\HP5\Methods\DS\_8015-C24T-JD-L#.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111Jd-C24-T.CAL  
 Sample Weight: 990 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.57 to 14.43

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	12.278	.202	.175	86.79
*1-Chlorooctadecane	29.972	.202	.	-
*#Triacontane	16.354	.202	.087	43.31

DRO Area:172804.6  
 TEH Area:427170.8

DRO Amount: 5.34195E-03  
 TEH Amount: 1.320523E-02




ERH2470 (RHMW19)

G:\org\HP5\DAT\HP5012722\_b\0127HP5.0012.RAW

Batch ID: 163190

B22011446-001D ;0127HP5 , \$HC-8015-DRO-W, SGT



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: B22011446-001D ;0127HP5 , \$HC-8015-DRO-W, SGT  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0012.RAW  
 Date & Time Acquired: 1/27/2022 4:21:39 PM  
 Method File: G:\Org\HP5\Methods\DR\_8015-C24T-JD-L%.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JD-C24-T.CAL  
 Sample Weight: 1010 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.57 to 14.43

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC		
*o-Terphenyl	12.278	.198	.171	86.26	-	
*1-Chlorooctadecane	13.134	.198	.	.04	-	
*#Triacontane	16.35	.198	.086	43.35	-	


DRO Area:235639.9 DRO Amount: 7.140147E-03  
 TEH Area:514117.2 TEH Amount: 1.557831E-02

ERH2470 (RHMW19)

Batch ID: 163190

G:\org\HP5\DAT\HP5012722\_b\0127HP5.0012.RAW

B22011446-001D ;0127HP5 , \$HC-8015-DRO-W, SGT



**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: B22011446-001D ;0127HP5 , \$HC-8015-DRO-W, SGT  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0012.RAW  
 Date & Time Acquired: 1/27/2022 4:21:39 PM  
 Method File: G:\Org\HP5\Methods\DR\_OROS-BD-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BD\_SAMP.CAL  
 Sample Weight: 1010 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 26424.55  
 Rt range for Residual Range Organics: 14.33 to 21.83

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*#Triacontane_____	16.35	.495	.086	17.34


RRO Area:221269.8 RRO AMOUNT: 8.290736E-03

ERH2470 (RHMW19)

Batch ID: 163190

G:\org\HP5\DAT\HP5012722\_b\0127HP5.0012.RAW

B22011446-001D ;0127HP5 , \$HC-8015-DRO-W, SGT



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: B22011446-001D ;0127HP5 , \$HC-8015-DRO-W, SGT  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0012.RAW  
 Date & Time Acquired: 1/27/2022 4:21:39 PM  
 Method File: G:\Org\HP5\Methods\DS\_8015-C24T-JD-L#.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO2201111Jd-C24-T.CAL  
 Sample Weight: 1010 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.57 to 14.43

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	12.278	.198	.171	86.14
*1-Chlorooctadecane	13.134	.198	.	.02
*#Triacontane	16.35	.198	.085	43.17


DRO Area:165042.5 DRO Amount: 5.000968E-03  
 TEH Area:449698.9 TEH Amount: 1.362637E-02

ERH2439 (RHMW2254-01 LF)

Batch ID: 163190

G:\org\HP5\DAT\HP5012722\_b\0127HP5.0013.RAW

B22011446-017D ;0127HP5 , \$HC-8015-DRO-W, SGT



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: B22011446-017D ;0127HP5 , \$HC-8015-DRO-W, SGT  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0013.RAW  
 Date & Time Acquired: 1/27/2022 5:04:14 PM  
 Method File: G:\Org\HP5\Methods\DR\_8015-C24T-JD-L%.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JD-C24-T.CAL  
 Sample Weight: 1030 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.57 to 14.43

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.279	.194	.182	93.55	-
*1-Chlorooctadecane	13.132	.194	.	.04	-
*#Triacontane	16.351	.194	.086	44.53	-


DRO Area:834081.8 DRO Amount: 2.478284E-02  
 TEH Area:1102743 TEH Amount: 3.276548E-02

ERH2439 (RHMW2254-01 LF)

Batch ID: 163190

G:\org\HP5\DAT\HP5012722\_b\0127HP5.0013.RAW

B22011446-017D ;0127HP5 , \$HC-8015-DRO-W, SGT



**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: B22011446-017D ;0127HP5 , \$HC-8015-DRO-W, SGT  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0013.RAW  
 Date & Time Acquired: 1/27/2022 5:04:14 PM  
 Method File: G:\Org\HP5\Methods\DR\_OROS-BD-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BD\_SAMP.CAL  
 Sample Weight: 1030 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 26424.55  
 Rt range for Residual Range Organics: 14.33 to 21.83

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*#Triacontane_____	16.351	.485	.086	17.81


RRO Area:145101.8 RRO AMOUNT: 5.331235E-03

ERH2439 (RHMW2254-01 LF)

Batch ID: 163190

G:\org\HP5\DAT\HP5012722\_b\0127HP5.0013.RAW

B22011446-017D ;0127HP5 , \$HC-8015-DRO-W, SGT



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**


Sample Name: B22011446-017D ;0127HP5 , \$HC-8015-DRO-W, SGT  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0013.RAW  
 Date & Time Acquired: 1/27/2022 5:04:14 PM  
 Method File: G:\Org\HP5\Methods\DS\_8015-C24T-JD-L#.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO2201111Jd-C24-T.CAL  
 Sample Weight: 1030 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.57 to 14.43

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.279	.194	.181	93.33	-
*1-Chlorooctadecane	13.132	.194	.	.01	-
*#Triacontane	16.351	.194	.086	44.29	-

DRO Area:355811 DRO Amount: 1.057211E-02  
 TEH Area:660338.9 TEH Amount: 1.962047E-02



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: DCM-Baseline Check-V14  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0014.RAW  
 Date & Time Acquired: 1/27/2022 5:47:00 PM  
 Method File: G:\Org\HP5\Methods\DR\_8015-JA-LEXP.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JA.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36  
 Rt range for Diesel Range Organics: 6.63 to 15.99

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.304	200.	.193	.1	-
*1-Chlorooctadecane	29.976	200.	.	.	-

DRO Area:341937.8 DRO Amount: 10.4647  
 TEH Area:457093.1 TEH Amount: 13.98892




ERH2442 (Sump Adit3)

G:\org\HP5\DAT\HP5012722\_b\0127HP5.0015.RAW

Batch ID: 163190

B22011446-022D ;0127HP5 , \$HC-8015-DRO-W, SGT



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: B22011446-022D ;0127HP5 , \$HC-8015-DRO-W, SGT  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0015.RAW  
 Date & Time Acquired: 1/27/2022 6:29:45 PM  
 Method File: G:\Org\HP5\Methods\D3\_8015-C24T-JD-L%.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JD-C24-T.CAL  
 Sample Weight: 1020 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.57 to 14.43

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.277	.196	.179	91.33	-
*1-Chlorooctadecane	13.131	.196	.	.05	-
*#Triacontane	16.35	.196	.093	47.66	-

DRO Area: 2.192973E+07 DRO Amount: 0.6579801


TEH Area: 2.63767E+07 TEH Amount: 0.791407

ERH2442 (Sump Adit3)

Batch ID: 163190

G:\org\HP5\DAT\HP5012722\_b\0127HP5.0015.RAW

B22011446-022D ;0127HP5 , \$HC-8015-DRO-W, SGT



**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: B22011446-022D ;0127HP5 , \$HC-8015-DRO-W, SGT  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0015.RAW  
 Date & Time Acquired: 1/27/2022 6:29:45 PM  
 Method File: G:\Org\HP5\Methods\D3\_OROS-BD-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BD\_SAMP.CAL  
 Sample Weight: 1020 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 26424.55  
 Rt range for Residual Range Organics: 14.33 to 21.83

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*#Triacontane_____	16.35	.49	.093	19.06	-


RRO Area:3423568 RRO AMOUNT: 0.1270197

ERH2442 (Sump Adit3)

Batch ID: 163190

G:\org\HP5\DAT\HP5012722\_b\0127HP5.0015.RAW

B22011446-022D ;0127HP5 , \$HC-8015-DRO-W, SGT



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: B22011446-022D ;0127HP5 , \$HC-8015-DRO-W, SGT  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0015.RAW  
 Date & Time Acquired: 1/27/2022 6:29:45 PM  
 Method File: G:\Org\HP5\Methods\DS\_8015-C24T-JD-L#.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111Jd-C24-T.CAL  
 Sample Weight: 1020 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.57 to 14.43

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.277	.196	.178	90.96	-
*1-Chlorooctadecane	13.131	.196	.	.02	-
*#Triacontane	16.35	.196	.087	44.51	-


DRO Area:1.771889E+07 DRO Amount: 0.531638  
 TEH Area:1.839462E+07 TEH Amount: 0.5519127

ERH2437 (RHMW2254-01 Bailer)

Batch ID: 163190

G:\org\HP5\DAT\HP5012722\_b\0127HP5.0016.RAW

B22011446-012B ;0127HP5 , \$HC-8015-DRO-W, SGT



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: B22011446-012B ;0127HP5 , \$HC-8015-DRO-W, SGT  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0016.RAW  
 Date & Time Acquired: 1/27/2022 7:12:32 PM  
 Method File: G:\Org\HP5\Methods\D3\_8015-012716-JD-L%.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JD-C24-T.CAL  
 Sample Weight: 1030 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.57 to 14.43

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.277	.194	.169	87.03	-
*1-Chlorooctadecane	13.156	.194	.	.09	-
*#Triacontane	16.351	.194	.088	45.52	-


DRO Area:2504376 DRO Amount: 7.441181E-02  
 TEH Area:6789349 TEH Amount: 0.20173

ERH2437 (RHMW2254-01 Bailer)

Batch ID: 163190

G:\org\HP5\DAT\HP5012722\_b\0127HP5.0016.RAW

B22011446-012B ;0127HP5 , \$HC-8015-DRO-W, SGT



**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: B22011446-012B ;0127HP5 , \$HC-8015-DRO-W, SGT  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0016.RAW  
 Date & Time Acquired: 1/27/2022 7:12:32 PM  
 Method File: G:\Org\HP5\Methods\D3\_OROS-012716-BD-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BD\_SAMP.CAL  
 Sample Weight: 1030 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 26424.55  
 Rt range for Residual Range Organics: 14.33 to 21.83

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*#Triacontane_____	16.351	.485	.088	18.21


RRO Area:3329877 RRO AMOUNT: 0.1223442

ERH2437 (RHMW2254-01 Bailer)

Batch ID: 163190

G:\org\HP5\DAT\HP5012722\_b\0127HP5.0016.RAW

B22011446-012B ;0127HP5 , \$HC-8015-DRO-W, SGT



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: B22011446-012B ;0127HP5 , \$HC-8015-DRO-W, SGT  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0016.RAW  
 Date & Time Acquired: 1/27/2022 7:12:32 PM  
 Method File: G:\Org\HP5\Methods\DS\_8015-C24T-JD-L#.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO2201111Jd-C24-T.CAL  
 Sample Weight: 1030 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.57 to 14.43

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	12.277	.194	.169	86.93
*1-Chlorooctadecane	13.156	.194	.07	-
*#Triacontane	16.351	.194	.085	43.72


DRO Area:1673816 DRO Amount: 4.973361E-02  
 TEH Area:1926903 TEH Amount: 5.725351E-02

ERH2435 (RHMW2254-01 Bailer)

Batch ID: 163190

G:\org\HP5\DAT\HP5012722\_b\0127HP5.0017.RAW

B22011446-011D ;0127HP5 , \$HC-8015-DRO-W, SGT



**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: B22011446-011D ;0127HP5 , \$HC-8015-DRO-W, SGT  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0017.RAW  
 Date & Time Acquired: 1/27/2022 7:55:16 PM  
 Method File: G:\Org\HP5\Methods\D3\_OROS-012717-BD-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BD\_SAMP.CAL  
 Sample Weight: 1010 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 26424.55  
 Rt range for Residual Range Organics: 14.33 to 21.83

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*#Triacontane_____	16.35	.495	.1	20.1 -


RRO Area:2121808 RRO AMOUNT: 0.0795018

ERH2435 (RHMW2254-01 Bailer)

Batch ID: 163190

G:\org\HP5\DAT\HP5012722\_b\0127HP5.0017.RAW

B22011446-011D ;0127HP5 , \$HC-8015-DRO-W, SGT



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: B22011446-011D ;0127HP5 , \$HC-8015-DRO-W, SGT  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0017.RAW  
 Date & Time Acquired: 1/27/2022 7:55:16 PM  
 Method File: G:\Org\HP5\Methods\DR\_8015-012717-JD-L%.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111Jd-C24-T.CAL  
 Sample Weight: 1010 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.57 to 14.43

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.276	.198	.133	67.09	-
*1-Chlorooctadecane	13.133	.198	.	.14	-
*#Triacontane	16.35	.198	.1	50.25	-

DRO Area:2440933 DRO Amount: 7.396293E-02  
 TEH Area:4915867 TEH Amount: 0.1489561




ERH2435 (RHMW2254-01 Bailer)

Batch ID: 163190

G:\org\HP5\DAT\HP5012722\_b\0127HP5.0017.RAW

B22011446-011D ;0127HP5 , \$HC-8015-DRO-W, SGT



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**


Sample Name: B22011446-011D ;0127HP5 , \$HC-8015-DRO-W, SGT  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0017.RAW  
 Date & Time Acquired: 1/27/2022 7:55:16 PM  
 Method File: G:\Org\HP5\Methods\DS\_8015-C24T-JD-L#.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO2201111Jd-C24-T.CAL  
 Sample Weight: 1010 Dilution: 1 S.A.: 1


Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.57 to 14.43

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.276	.198	.133	66.97	-
*1-Chlorooctadecane	13.133	.198	.	.02	-
*#Triacontane	16.35	.198	.098	49.3	-

DRO Area:1786952 DRO Amount: 5.414659E-02  
 TEH Area:2134540 TEH Amount: 6.467889E-02





**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: CCV\_0127HP519r, RRO ;0127HP5 , DRO220118A  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0019.RAW  
 Date & Time Acquired: 1/27/2022 9:20:37 PM  
 Method File: G:\Org\HP5\Methods\DC\_ORO-BD-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111Bd.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for for ~~Residual~~ TEH(Oil Range) Organics Calculations: 26424.55  
 Rt range for ~~Residual~~ TEH(Oil Range) Organics: 12.62 to 30.05

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*#Triacontane	16.356	500.	333.682	66.74	-

RRO TEH(Oil Range) Area:1.22113E+08 RRO TEH(Oil Range) AMOUNT: 4621.193


CONTINUING CALIBRATION REPORT: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0019.RAW

COMPOUND	ACTUAL (NG)	MEASURED (NG)	%RECOVERY	LIMITS
*30-40 Motor Oil	5000.	.039	.	75-125

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	LIMITS
*#Triacontane	16.356	200.	333.682	166.84	75-125

AMN 02/15/2022



**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: CCV\_0127HP519r, RRO ;0127HP5 , DRO220118A  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0019.RAW  
 Date & Time Acquired: 1/27/2022 9:20:37 PM  
 Method File: G:\Org\HP5\Methods\DS\_ORO-BD-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BD.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 26424.55  
 Rt range for Residual Range Organics: 12.62 to 30.05

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*#Triacontane	16.356	500.	211.762	42.35	-


RRO Area:2934929 RRO AMOUNT: 111.0683

**CONTINUING CALIBRATION REPORT: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0019.RAW**

COMPOUND	ACTUAL (NG)	MEASURED (NG)	%RECOVERY	LIMITS
*30-40 Motor Oil	5000.	.039	.	75-125

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	LIMITS
*#Triacontane	16.356	200.	211.762	105.88	75-125



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: CCV\_0127HP520r, DRO ;0127HP5 , DRO220124A  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0020.RAW  
 Date & Time Acquired: 1/27/2022 10:03:19 PM  
 Method File: G:\Org\HP5\Methods\DC\_8015-C24-JD-L%.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JD-C24.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36  
 Rt range for Diesel Range Organics: 6.57 to 14.43

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	12.284	200.	314.435	157.22
*1-Chlorooctadecane	13.128	200.	151.884	75.94

DRO Area: 4.60242E+08 DRO Amount: 14085.29  
 TEH Area: 4.764987E+08 TEH Amount: 14582.81


CONTINUING CALIBRATION REPORT: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0020.RAW

COMPOUND	ACTUAL (NG)	MEASURED (NG)	%RECOVERY	LIMITS
TOTAL DRO	15000.	14582.81	97.22	85-115

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	LIMITS
*o-Terphenyl	12.284	200.	314.435	157.22	85-115
*1-Chlorooctadecane	13.128	200.	151.884	75.94	85-115

G:\org\HP5\DAT\HP5012722\_b\0127HP5.0020.RAW

CCV\_0127HP520r, DRO ;0127HP5 , DRO220124A



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: CCV\_0127HP520r, DRO ;0127HP5 , DRO220124A  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0020.RAW  
 Date & Time Acquired: 1/27/2022 10:03:19 PM  
 Method File: G:\Org\HP5\Methods\DS\_8015-C24-JD-L#.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JD-C24.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.57 to 14.43


SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	12.284	200.	193.111	96.56
*1-Chlorooctadecane	13.128	200.	34.472	17.24

DRO Area: 2.390552E+08 DRO Amount: 7316.069  
 TEH Area: 2.497168E+08 TEH Amount: 7642.358

CONTINUING CALIBRATION REPORT: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0020.RAW

COMPOUND	ACTUAL (NG)	MEASURED (NG)	%RECOVERY	LIMITS
TOTAL DRO	15000.	7642.36	50.95	85-115

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	LIMITS
*o-Terphenyl	12.284	200.	193.111	96.56	85-115
*1-Chlorooctadecane	13.128	200.	34.472	17.24	85-115




**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: DCM-Baseline Check-V21  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0021.RAW  
 Date & Time Acquired: 1/27/2022 10:46:04 PM  
 Method File: G:\Org\HP5\Methods\DR\_8015-JA-LEXP.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JA.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36  
 Rt range for Diesel Range Organics: 6.63 to 15.99

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	29.859	200.	.	-
*1-Chlorooctadecane	29.859	200.	.	-

DRO Area:219039.1 DRO Amount: 6.703496  
 TEH Area:315262.3 TEH Amount: 9.64832



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: DCM-Baseline Check-V22  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0022.RAW  
 Date & Time Acquired: 1/27/2022 11:28:45 PM  
 Method File: G:\Org\HP5\Methods\DR\_8015-JA-LEXP.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JA.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36  
 Rt range for Diesel Range Organics: 6.63 to 15.99

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	29.959	200.	.407	.2
*1-Chlorooctadecane	13.163	200.		


DRO Area: 2515289 DRO Amount: 76.97814  
 TEH Area: 2910134 TEH Amount: 89.06203



Batch ID: 163190

B22011446-001DMS ;0127HP5 , SGT

G:\org\HP5\DAT\HP5012722\_b\0127HP5.0023.RAW



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: B22011446-001DMS ;0127HP5 , SGT  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0023.RAW  
 Date & Time Acquired: 1/28/2022 12:11:24 AM  
 Method File: G:\Org\HP5\Methods\D3\_8015-C24-JD-L%.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JD-C24.CAL  
 Sample Weight: 990 Dilution: 1 S.A.: 1


Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.57 to 14.43

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*o-Terphenyl	12.28	.202	.317	156.75	-
*1-Chlorooctadecane	13.129	.202	.134	66.32	-

DRO Area: 3.797233E+08 DRO Amount: 11.73847  
 TEH Area: 4.058049E+08 TEH Amount: 12.54474

Batch ID: 163190  
G:\org\HP5\DAT\HP5012722\_b\0127HP5.0023.RAW B22011446-001DMS ;0127HP5 , SGT




**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: B22011446-001DMS ;0127HP5 , SGT  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0023.RAW  
 Date & Time Acquired: 1/28/2022 12:11:24 AM  
 Method File: G:\Org\HP5\Methods\DS\_8015-C24-JD-L#.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JD-C24.CAL  
 Sample Weight: 990 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36  
 Rt range for Diesel Range Organics: 6.57 to 14.43

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	12.28	.202	.182	90.13
*1-Chlorooctadecane	13.129	.202	.051	25.17

DRO Area: 1.758424E+08 DRO Amount: 5.435858  
 TEH Area: 1.85976E+08 TEH Amount: 5.749119



**RESIDUAL RANGE ORGANICS CHROMATOGRAM**


Sample Name: B22011446-006DMS-RRO ;0127HP5 , SGT  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0024.RAW  
 Date & Time Acquired: 1/28/2022 12:54:00 AM  
 Method File: G:\Org\HP5\Methods\D3\_ORO-BD-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BD.CAL  
 Sample Weight: 1060 Dilution: 1 S.A.: 1

Mean RF for for ~~Residual~~ TEH(Oil Range) Organics Calculations: 26424.55  
 Rt range for ~~Residual~~ TEH(Oil Range) Organics: 12.62 to 30.05

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*#Triacontane	16.351	.472	.15	31.75	-

~~RRO~~ TEH(Oil Range) Area:1.210655E+08 ~~RRO~~ TEH(Oil Range) AMOUNT: 4.322219

AMN 02/15/2022




**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: B22011446-006DMS-RRO ;0127HP5 , SGT  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0024.RAW  
 Date & Time Acquired: 1/28/2022 12:54:00 AM  
 Method File: G:\Org\HP5\Methods\DS\_ORO-BD-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BD.CAL  
 Sample Weight: 1060 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 26424.55  
 Rt range for Residual Range Organics: 12.62 to 30.05

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*#Triacontane_____	16.351	.472	.078	16.49

RRO Area:2305464 RRO AMOUNT: 8.230852E-02



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**


Sample Name: DCM-Baseline Check-V25  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0025.RAW  
 Date & Time Acquired: 1/28/2022 1:36:38 AM  
 Method File: G:\Org\HP5\Methods\DR\_8015-JA-LEXP.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JA.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.63 to 15.99

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	12.302	200.	.107	.05
*1-Chlorooctadecane	29.73	200.	.	.

DRO Area:291135 DRO Amount: 8.909925  
 TEH Area:820673.9 TEH Amount: 25.11599



**RESIDUAL RANGE ORGANICS CHROMATOGRAM**


Sample Name: LCS-163190-RRO ;0127HP5 , SGT  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0026.RAW  
 Date & Time Acquired: 1/28/2022 2:19:19 AM  
 Method File: G:\Org\HP5\Methods\D3\_ORO-BD-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BD.CAL  
 Sample Weight: 1000 Dilution: 1 S.A.: 1


Mean RF for for ~~Residual~~ TEH(Oil Range) Organics Calculations: 26424.55  
 Rt range for ~~Residual~~ TEH(Oil Range) Organics: 12.62 to 30.05

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*#Triacontane	16.353	.5	.179	35.79

RRO TEH(Oil Range) Area:1.320924E+08 RRO TEH(Oil Range) AMOUNT: 4.998849

AMN 02/15/2022





**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: DCM-Baseline Check-V27  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0027.RAW  
 Date & Time Acquired: 1/28/2022 3:01:52 AM  
 Method File: G:\Org\HP5\Methods\DR\_8015-JA-LEXP.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JA.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1


Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.63 to 15.99

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	12.304	200.	.098	.05
*1-Chlorooctadecane	29.771	200.	.	.

DRO Area: 209355.9 DRO Amount: 6.40715  
 TEH Area: 678923.1 TEH Amount: 20.77783





**RESIDUAL RANGE ORGANICS CHROMATOGRAM**


Sample Name: LCSD-163190-RRO ;0127HP5 , SGT  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0028.RAW  
 Date & Time Acquired: 1/28/2022 3:44:28 AM  
 Method File: G:\Org\HP5\Methods\D3\_ORO-BD-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BD.CAL  
 Sample Weight: 1000 Dilution: 1 S.A.: 1

Mean RF for for ~~Residual~~ TEH(Oil Range) Organics Calculations: 26424.55  
 Rt range for ~~Residual~~ TEH(Oil Range) Organics: 12.62 to 30.05

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*#Triacontane	16.354	.5	.196	39.16

~~RRO~~ TEH(Oil Range) Area:1.292734E+08 ~~RRO~~ TEH(Oil Range) AMOUNT: 4.89217

AMN 02/15/2022




**RESIDUAL RANGE ORGANICS CHROMATOGRAM**


Sample Name: LCSD-163190-RRO ;0127HP5 , SGT  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0028.RAW  
 Date & Time Acquired: 1/28/2022 3:44:28 AM  
 Method File: G:\Org\HP5\Methods\DS\_ORO-BD-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BD.CAL  
 Sample Weight: 1000 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 26424.55  
 Rt range for Residual Range Organics: 12.62 to 30.05

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*#Triacontane	16.354	.5	.091	18.13

RRO Area:2807590 RRO AMOUNT: 0.1062493





**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: CCV\_0127HP530r, RRO ;0127HP5 , DRO220118A  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0030.RAW  
 Date & Time Acquired: 1/28/2022 5:09:42 AM  
 Method File: G:\Org\HP5\Methods\DC\_ORO-BD-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111Bd.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for for ~~Residual~~ TEH(Oil Range) Organics Calculations: 26424.55  
 Rt range for ~~Residual~~ TEH(Oil Range) Organics: 12.62 to 30.05

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*#Triacontane	16.356	500.	350.681	70.14	-

~~RRO~~ TEH(Oil Range) Area:1.287033E+08 ~~RRO~~ TEH(Oil Range) AMOUNT: 4870.594


CONTINUING CALIBRATION REPORT: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0030.RAW

COMPOUND	ACTUAL (NG)	MEASURED (NG)	%RECOVERY	LIMITS
*30-40 Motor Oil	5000.	.028	.	75-125

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	LIMITS
*#Triacontane	16.356	200.	350.681	175.34	75-125

AMN 02/15/2022



**RESIDUAL RANGE ORGANICS CHROMATOGRAM**

Sample Name: CCV\_0127HP530r, RRO ;0127HP5 , DRO220118A  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0030.RAW  
 Date & Time Acquired: 1/28/2022 5:09:42 AM  
 Method File: G:\Org\HP5\Methods\DS\_ORO-BD-L%.MET  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_ORO220111BD.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for for Residual Range Organics Calculations: 26424.55  
 Rt range for Residual Range Organics: 12.62 to 30.05


SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	
*#Triacontane	16.356	500.	218.544	43.71	-

RRO Area:3164239 RRO AMOUNT: 119.7462

CONTINUING CALIBRATION REPORT: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0030.RAW

COMPOUND	ACTUAL (NG)	MEASURED (NG)	%RECOVERY	LIMITS
*30-40 Motor Oil	5000.	.028	.	75-125

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	LIMITS
*#Triacontane	16.356	200.	218.544	109.27	75-125



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: CCV\_0127HP531r, DRO ;0127HP5 , DRO220124A  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0031.RAW  
 Date & Time Acquired: 1/28/2022 5:52:23 AM  
 Method File: G:\Org\HP5\Methods\DC\_8015-C24-JD-L%.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JD-C24.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36  
 Rt range for Diesel Range Organics: 6.57 to 14.43

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	12.282	200.	300.622	150.31
*1-Chlorooctadecane	13.127	200.	143.801	71.9

DRO Area: 4.37416E+08 DRO Amount: 13386.72  
 TEH Area: 4.527705E+08 TEH Amount: 13856.63


CONTINUING CALIBRATION REPORT: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0031.RAW

COMPOUND	ACTUAL (NG)	MEASURED (NG)	%RECOVERY	LIMITS
TOTAL DRO	15000.	13856.63	92.38	85-115

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	LIMITS
*o-Terphenyl	12.282	200.	300.622	150.31	85-115
*1-Chlorooctadecane	13.127	200.	143.801	71.9	85-115

G:\org\HP5\DAT\HP5012722\_b\0127HP5.0031.RAW

CCV\_0127HP531r, DRO ;0127HP5 , DRO220124A



**DIESEL RANGE ORGANICS CHROMATOGRAM REPORT**

Sample Name: CCV\_0127HP531r, DRO ;0127HP5 , DRO220124A  
 Raw File: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0031.RAW  
 Date & Time Acquired: 1/28/2022 5:52:23 AM  
 Method File: G:\Org\HP5\Methods\DS\_8015-C24-JD-L#.met  
 Calibration File: G:\Org\HP5\Cals\SW8015C\_DRO220111JD-C24.CAL  
 Sample Weight: 1 Dilution: 1 S.A.: 1

Mean RF for TEH: 32675.36

Rt range for Diesel Range Organics: 6.57 to 14.43

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC
*o-Terphenyl	12.282	200.	183.74	91.87
*1-Chlorooctadecane	13.127	200.	33.176	16.59

DRO Area: 2.268986E+08 DRO Amount: 6944.028  
 TEH Area: 2.369893E+08 TEH Amount: 7252.844

CONTINUING CALIBRATION REPORT: G:\org\HP5\DAT\HP5012722\_b\0127HP5.0031.RAW

COMPOUND	ACTUAL (NG)	MEASURED (NG)	%RECOVERY	LIMITS
TOTAL DRO	15000.	7252.84	48.35	85-115

SURROGATE COMPOUND	RT	ACTUAL	MEASURED	%REC	LIMITS
*o-Terphenyl	12.282	200.	183.74	91.87	85-115
*1-Chlorooctadecane	13.127	200.	33.176	16.59	85-115

Write Sequence	Data File	Sample Name	Method	Weight	Dil Factor	Amt Inj	IS	Cal ID	Manual Integrations
G:\org\HP5\DAT\HP5012422_b\0124HP5.52	MARKER_0124HP552r_DRO_0124HP5_DRO220111A		G:\org\HP5\Methods\CSC220124.met	1	1	1	1	0	No Integrations
G:\org\HP5\DAT\HP5012422_b\0124HP5.53	GCV_0124HP553r_RRO_0124HP5_DRO220118A		G:\org\HP5\Methods\DC_ORO-BC-L%.MET G:\org\HP5\Methods\DS_ORO-BC-L%.MET	1	1	1	1	0	The integration of Oil Range hydrocarbon is the hydrocarbon response with reference to the baseline. Surrogates are integrated using a valley to valley integration using Set Baseline All Valleys on placed at 15.14 minutes and X-axis scaling showing surrogate peak from 14-18 minutes.
G:\org\HP5\DAT\HP5012422_b\0124HP5.54	GCV_0124HP554r_DRO_0124HP5_DRO220124A		G:\org\HP5\Methods\DC_8015-C24-JC-L%.met G:\org\HP5\Methods\DS_8015-C24-JC-L%.met	1	1	1	1	0	The integration of Diesel Range Organics (C10-C24) and Total Extractable Hydrocarbons is the hydrocarbon response with reference to the baseline. Assigned Set Baseline All Valley on at 16.35 minutes. Surrogates are integrated using a valley to valley integration using Set Baseline All Valleys on placed at 12.01 minutes and X-axis scaling showing surrogate peak from 11.5-14 minutes.
G:\org\HP5\DAT\HP5012422_b\0124HP5.55	DCM-Baseline Check-V54		G:\org\HP5\Methods\DR_8015-JA-LEXP.met	1	1	1	1	0	No Integrations
G:\org\HP5\DAT\HP5012422_b\0124HP5.56	LCS-163190_0124HP5		G:\org\HP5\Methods\D3_8015-C24-JC-L%.met G:\org\HP5\Methods\DS_8015-C24-JC-L%.met	1000	1	1	1	0	The integration of Diesel Range Organics (C10-C24) and Total Extractable Hydrocarbons is the hydrocarbon response with reference to the baseline. Surrogates are integrated using a valley to valley integration using Set Baseline All Valleys on placed at 12.01 minutes and X-axis scaling showing surrogate peak from 11.5-14 minutes.
G:\org\HP5\DAT\HP5012422_b\0124HP5.57	LCS2-163190_0124HP5		G:\org\HP5\Methods\D3_8015-C24-JC-L%.met G:\org\HP5\Methods\DS_8015-C24-JC-L%.met	1000	1	1	1	0	The integration of Diesel Range Organics (C10-C24) and Total Extractable Hydrocarbons is the hydrocarbon response with reference to the baseline. Surrogates are integrated using a valley to valley integration using Set Baseline All Valleys on placed at 12.01 minutes and X-axis scaling showing surrogate peak from 11.5-14 minutes.
G:\org\HP5\DAT\HP5012422_b\0124HP5.58	MB-163190_0124HP5		G:\org\HP5\Methods\DR_8015-C24-JC-L%.met G:\org\HP5\Methods\DR_OROS-BC-L%.MET G:\org\HP5\Methods\DS_8015-C24-JC-L%.met	1000	1	1	1	0	The integration of Diesel Range Organics (C10-C24), C24-C40, and Total Extractable Hydrocarbons (TEH) is the hydrocarbon response with reference to the baseline. Assigned Set Baseline All Valley on at 17.12 minutes. Surrogates are integrated using a valley to valley integration using Set Baseline All Valleys on at 10.78 minutes and X-axis scaling showing surrogate peak from 11-18 minutes.
G:\org\HP5\DAT\HP5012422_b\0124HP5.59	B22011446-006D_0124HP5_SHC-8015-DRO-W		G:\org\HP5\Methods\DR_8015-C24-JC-L%.met G:\org\HP5\Methods\DR_OROS-BC-L%.MET G:\org\HP5\Methods\DS_8015-C24-JC-L%.met	990	1	1	1	0	The integration of Diesel Range Organics (C10-C24), C24-C40, and Total Extractable Hydrocarbons (TEH) is the hydrocarbon response with reference to the baseline. Assigned Set Baseline All Valley on at 10.78 minutes and X-axis scaling showing surrogate peak from 11-18 minutes.
G:\org\HP5\DAT\HP5012422_b\0124HP5.60	B22011446-017D_0124HP5_SHC-8015-DRO-W		G:\org\HP5\Methods\D3_8015-012460-JC-L%.met G:\org\HP5\Methods\DR_OROS-BC-L%.MET G:\org\HP5\Methods\DS_8015-C24-JC-L%.met	1030	1	1	1	0	The integration of Diesel Range Organics (C10-C24), C24-C40, and Total Extractable Hydrocarbons (TEH) is the hydrocarbon response with reference to the baseline with peak width adjusted. Surrogates are integrated using a valley to valley integration using Set Baseline All Valleys on at 10.78 minutes and X-axis scaling showing surrogate peak from 11-18 minutes.
G:\org\HP5\DAT\HP5012422_b\0124HP5.61	B22011446-027D_0124HP5_SHC-8015-DRO-W_Needs RR due to possible carry over		G:\org\HP5\Methods\DR_8015-C24-JC-L%.met	1040	1	1	1	0	No Integrations
G:\org\HP5\DAT\HP5012422_b\0124HP5.62	DCM-Baseline Check-V82		G:\org\HP5\Methods\DR_8015-JA-LEXP.met	1	1	1	1	0	No Integrations
G:\org\HP5\DAT\HP5012422_b\0124HP5.63	B22011446-022D_0124HP5_SHC-8015-DRO-W		G:\org\HP5\Methods\D3_8015-C24-JC-L%.met G:\org\HP5\Methods\DR_OROS-BC-L%.MET G:\org\HP5\Methods\DS_8015-C24-JC-L%.met	1020	1	1	1	0	The integration of Diesel Range Organics (C10-C24), C24-C40, and Total Extractable Hydrocarbons (TEH) is the hydrocarbon response with reference to the baseline. Surrogates are integrated using a valley to valley integration using Set Baseline All Valleys on at 10.78 minutes and X-axis scaling showing surrogate peak from 11-18 minutes.
G:\org\HP5\DAT\HP5012422_b\0124HP5.64	B22011446-012B_0124HP5_SHC-8015-DRO-W		G:\org\HP5\Methods\D3_8015-C24-JC-L%.met G:\org\HP5\Methods\DR_OROS-BC-L%.MET G:\org\HP5\Methods\DS_8015-C24-JC-L%.met	1030	1	1	1	0	The integration of Diesel Range Organics (C10-C24), C24-C40, and Total Extractable Hydrocarbons (TEH) is the hydrocarbon response with reference to the baseline. Surrogates are integrated using a valley to valley integration using Set Baseline All Valleys on at 10.78 minutes and X-axis scaling showing surrogate peak from 11-18 minutes.
G:\org\HP5\DAT\HP5012422_b\0124HP5.65	B22011446-011D_0124HP5_SHC-8015-DRO-W		G:\org\HP5\Methods\D3_8015-C24-JC-L%.met G:\org\HP5\Methods\DR_OROS-BC-L%.MET G:\org\HP5\Methods\DS_8015-C24-JC-L%.met	1010	1	1	1	0	The integration of Diesel Range Organics (C10-C24), C24-C40, and Total Extractable Hydrocarbons (TEH) is the hydrocarbon response with reference to the baseline. Surrogates are integrated using a valley to valley integration using Set Baseline All Valleys on at 10.78 minutes and X-axis scaling showing surrogate peak from 11-18 minutes.
G:\org\HP5\DAT\HP5012422_b\0124HP5.66	DCM-Baseline Check-V66		G:\org\HP5\Methods\DR_8015-JA-LEXP.met	1	1	1	1	0	No Integrations
G:\org\HP5\DAT\HP5012422_b\0124HP5.67	B22011446-032D_0124HP5_SHC-8015-DRO-W		G:\org\HP5\Methods\DR_8015-C24-JC-L%.met G:\org\HP5\Methods\DR_OROS-BC-L%.MET G:\org\HP5\Methods\DS_8015-C24-JC-L%.met	990	1	1	1	0	The integration of Diesel Range Organics (C10-C24), C24-C40, and Total Extractable Hydrocarbons (TEH) is the hydrocarbon response with reference to the baseline. Assigned Set Baseline All Valley on at 17.12 minutes. Surrogates are integrated using a valley to valley integration using Set Baseline All Valleys on at 10.78 minutes and X-axis scaling showing surrogate peak from 11-18 minutes.
G:\org\HP5\DAT\HP5012422_b\0124HP5.68	MARKER_0124HP568r_DRO_0124HP5_DRO220111A		G:\org\HP5\Methods\CSC220124.met	1	1	1	1	0	No Integrations
G:\org\HP5\DAT\HP5012422_b\0124HP5.69	GCV_0124HP569r_RRO_0124HP5_DRO220118A		G:\org\HP5\Methods\DC_ORO-BC-L%.MET G:\org\HP5\Methods\DS_ORO-BC-L%.MET	1	1	1	1	0	The integration of Oil Range hydrocarbon is the hydrocarbon response with reference to the baseline. Surrogates are integrated using a valley to valley integration using Set Baseline All Valleys on placed at 15.14 minutes and X-axis scaling showing surrogate peak from 14-18 minutes.



G:\org\HP5\DAT\HP5012422_b\0124HP5.70	CCV_0124HP570r, DRO_0124HP5 , DRO220124A	G:\Org\HP5\Methods\DC_8015-C24-JC-L%.met G:\Org\HP5\Methods\DS_8015-C24-JC-L%.met	1	1	1	1	0	The integration of Diesel Range Organics (C10-C24) and Total Extractable Hydrocarbons is the hydrocarbon response with reference to the baseline. Assigned Set Baseline All Valley on at 16.35 minutes. Surrogates are integrated using a valley to valley integration using Set Baseline All Valleys on placed at 12.01 minutes and X-axis scaling showing surrogate peak from 11.5-14 minutes.
G:\org\HP5\DAT\HP5012422_b\0124HP5.71	DCM-Baseline Check-V71	G:\Org\HP5\Methods\DR_8015-JA-LEXP.met	1	1	1	1	0	No Integrations
G:\org\HP5\DAT\HP5012422_b\0124HP5.72	DCM-Baseline Check-V72	G:\Org\HP5\Methods\DR_8015-JA-LEXP.met	1	1	1	1	0	No Integrations
G:\org\HP5\DAT\HP5012422_b\0124HP5.73	B22011446-001D_0124HP5 , \$HC-8015-DRO-W,	G:\Org\HP5\Methods\D3_8015-C24-JC-L%.met G:\Org\HP5\Methods\D3_OROS-BC-L%.MET G:\Org\HP5\Methods\DS_8015-C24-JC-L%.met	1010	1	1	1	0	The integration of Diesel Range Organics (C10-C24), C24-C40, and Total Extractable Hydrocarbons (TEH) is the hydrocarbon response with reference to the baseline. Surrogates are integrated using a valley to valley integration using Set Baseline All Valleys on at 10.78 minutes and X-axis scaling showing surrogate peak from 11-18 minutes.
G:\org\HP5\DAT\HP5012422_b\0124HP5.74	B22011446-027D_0124HP5 , \$HC-8015-DRO-W, RR	G:\Org\HP5\Methods\DR_8015-C24-JC-L%.met G:\Org\HP5\Methods\DR_OROS-BC-L%.MET G:\Org\HP5\Methods\DS_8015-C24-JC-L%.met	1040	1	1	1	0	The integration of Diesel Range Organics (C10-C24), C24-C40, and Total Extractable Hydrocarbons (TEH) is the hydrocarbon response with reference to the baseline. Assigned Set Baseline All Valley on at 17.12 minutes. Surrogates are integrated using a valley to valley integration using Set Baseline All Valleys on at 10.78 minutes and X-axis scaling showing surrogate peak from 11-18 minutes.
G:\org\HP5\DAT\HP5012422_b\0124HP5.75	B22011446-001DMS_0124HP5 ,	G:\Org\HP5\Methods\D3_8015-012475-JC-L%.met G:\Org\HP5\Methods\DS_8015-C24-JC-L%.met	990	1	1	1	0	The integration of Diesel Range Organics (C10-C24) and Total Extractable Hydrocarbons is the hydrocarbon response with reference to the baseline with peak width adjusted. Surrogates are integrated using a valley to valley integration using Set Baseline All Valleys on placed at 12.01 minutes and X-axis scaling showing surrogate peak from 11.5-14 minutes.
G:\org\HP5\DAT\HP5012422_b\0124HP5.76	B22011446-006DMS-RR0_0124HP5 ,	G:\Org\HP5\Methods\D3_ORO-BC-L%.MET G:\Org\HP5\Methods\DS_ORO-BC-L%.MET	1060	1	1	1	0	The integration of Oil Range hydrocarbon is the hydrocarbon response with reference to the baseline. Surrogates are integrated using a valley to valley integration using Set Baseline All Valleys on placed at 16.14 minutes and X-axis scaling showing surrogate peak from 14-18 minutes.
G:\org\HP5\DAT\HP5012422_b\0124HP5.77	DCM-Baseline Check-V78	G:\Org\HP5\Methods\DR_8015-JA-LEXP.met	1	1	1	1	0	No Integrations
G:\org\HP5\DAT\HP5012422_b\0124HP5.78	LCS-163190-RR0_0124HP5 ,	G:\Org\HP5\Methods\D3_ORO-BC-L%.MET G:\Org\HP5\Methods\DS_ORO-BC-L%.MET	1000	1	1	1	0	The integration of Oil Range hydrocarbon is the hydrocarbon response with reference to the baseline. Surrogates are integrated using a valley to valley integration using Set Baseline All Valleys on placed at 16.14 minutes and X-axis scaling showing surrogate peak from 14-18 minutes.
G:\org\HP5\DAT\HP5012422_b\0124HP5.79	DCM-Baseline Check-V80	G:\Org\HP5\Methods\DR_8015-JA-LEXP.met	1	1	1	1	0	No Integrations
G:\org\HP5\DAT\HP5012422_b\0124HP5.80	LCS0-163190-RR0_0124HP5 ,	G:\Org\HP5\Methods\D3_ORO-BC-L%.MET G:\Org\HP5\Methods\DS_ORO-BC-L%.MET	1000	1	1	1	0	The integration of Oil Range hydrocarbon is the hydrocarbon response with reference to the baseline. Surrogates are integrated using a valley to valley integration using Set Baseline All Valleys on placed at 16.14 minutes and X-axis scaling showing surrogate peak from 14-18 minutes.
G:\org\HP5\DAT\HP5012422_b\0124HP5.81	MARKER_0124HP582r, DRO_0124HP5 , DRO220111A	G:\org\HP5\Methods\CS0220124.met	1	1	1	1	0	No Integrations
G:\org\HP5\DAT\HP5012422_b\0124HP5.82	CCV_0124HP583r, RRO_0124HP5 , DRO220118A	G:\Org\HP5\Methods\DC_ORO-BC-L%.MET G:\Org\HP5\Methods\DS_ORO-BC-L%.MET	1	1	1	1	0	The integration of Oil Range hydrocarbon is the hydrocarbon response with reference to the baseline. Surrogates are integrated using a valley to valley integration using Set Baseline All Valleys on placed at 16.14 minutes and X-axis scaling showing surrogate peak from 14-18 minutes.
G:\org\HP5\DAT\HP5012422_b\0124HP5.83	CCV_0124HP584r, DRO_0124HP5 , DRO220124A	G:\Org\HP5\Methods\DC_8015-C24-JC-L%.met G:\Org\HP5\Methods\DS_8015-C24-JC-L%.met	1	1	1	1	0	The integration of Diesel Range Organics (C10-C24) and Total Extractable Hydrocarbons is the hydrocarbon response with reference to the baseline. Assigned Set Baseline All Valley on at 16.35 minutes. Surrogates are integrated using a valley to valley integration using Set Baseline All Valleys on placed at 12.01 minutes and X-axis scaling showing surrogate peak from 11.5-14 minutes.

*Ann Nebel*

Digitally signed by  
Ann Nebel  
Date: 2022.02.15 16:24:56 -07:00



G:\org\HP5\DAT\HP5012722_b\0127HP5.25r G:\org\HP5\DAT\HP5012722_b\0127HP5.26r	DCM-Baseline Check-V25 LCS-163190-RRO ;0127HP5 , SGT	G:\Org\HP5\Methods\DR_8015-JA-LEXP.met G:\Org\HP5\Methods\D3_ORO-BD-L%.MET G:\Org\HP5\Methods\DS_ORO-BD-L%.MET	1000	1	1	1	1	0	No integrations The integration of Oil Range hydrocarbon is the hydrocarbon response with reference to the baseline. Surrogates are integrated using a valley to valley integration using Set Baseline All Valleys on placed at 16.14 minutes and X-axis scaling showing surrogate peak from 14-18 minutes.
G:\org\HP5\DAT\HP5012722_b\0127HP5.27r G:\org\HP5\DAT\HP5012722_b\0127HP5.28r	DCM-Baseline Check-V27 LCS-163190-RRO ;0127HP5 , SGT	G:\Org\HP5\Methods\DR_8015-JA-LEXP.met G:\Org\HP5\Methods\D3_ORO-BD-L%.MET G:\Org\HP5\Methods\DS_ORO-BD-L%.MET	1000	1	1	1	1	0	No integrations The integration of Oil Range hydrocarbon is the hydrocarbon response with reference to the baseline. Surrogates are integrated using a valley to valley integration using Set Baseline All Valleys on placed at 16.14 minutes and X-axis scaling showing surrogate peak from 14-18 minutes.
G:\org\HP5\DAT\HP5012722_b\0127HP5.29r G:\org\HP5\DAT\HP5012722_b\0127HP5.28r	MARKER ;0127HP529r, DRO ;0127HP5 , DRO220111A CCV_0127HP530r, RRO ;0127HP5 , DRO220118A	G:\org\HP5\Methods\CSC220127.met G:\Org\HP5\Methods\DC_ORO-BD-L%.MET G:\Org\HP5\Methods\DS_ORO-BD-L%.MET		1	1	1	1	0	No integrations The integration of Oil Range hydrocarbon is the hydrocarbon response with reference to the baseline. Surrogates are integrated using a valley to valley integration using Set Baseline All Valleys on placed at 16.14 minutes and X-axis scaling showing surrogate peak from 14-18 minutes.
G:\org\HP5\DAT\HP5012722_b\0127HP5.31r	CCV_0127HP531r, DRO ;0127HP5 , DRO220124A	G:\Org\HP5\Methods\DC_8015-C24-JD-L%.met G:\Org\HP5\Methods\DS_8015-C24-JD-Lf%.met		1	1	1	1	0	The integration of Diesel Range Organics (C10-C24) and Total Extractable Hydrocarbons is the hydrocarbon response with reference to the baseline. Assigned Set Baseline All Valley on at 16.35 minutes. Surrogates are integrated using a valley to valley integration using Set Baseline All Valleys on placed at 12.01 minutes and X-axis scaling showing surrogate peak from 11.5-14 minutes.

*Ann Nebel*

Digitally signed by  
Ann Nebel  
Date: 2022.02.15 16:25:19 -07:00



# Analytical RunID GCFID-HP5-B\_220111A Standards Traceability Report

**Standard ID:** DRO180126C

**Standard Name:** 2-Fluorobiphenyl

**Prep Date:** 1/26/2018

**Exp Date:** 10/31/2024

**Department:** dropr

**Vendor:** Chemservice

**Lot Number:** 5599700

**Balance ID:**

**Comments:**

**Type:** Neat

**Prep By:** Todd C Cooper

**Status:** New

**Final Volume:** mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
2-Fluorobiphenyl	<a href="#">10069</a>		mL	10/31/2024
Stock Source	Base Units	Amount Added		



# Analytical RunID GCFID-HP5-B\_220111A Standards Traceability Report

**Standard ID:** DRO180823A

**Standard Name:** 2-Bromonaphthalene

**Prep Date:** 8/22/2016

**Exp Date:** 5/31/2022

**Department:** dropr

**Vendor:** Chemservice

**Lot Number:** 3150700

**Balance ID:**

**Comments:**

**Type:** Neat

**Prep By:** Ann Nebel

**Status:** New

**Final Volume:** mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
2-Bromonaphthalene	<a href="#">10701</a>		mL	5/31/2022
Stock Source	Base Units	Amount Added		



# Analytical RunID GCFID-HP5-B\_220111A Standards Traceability Report

**Standard ID:** DRO181105A

**Standard Name:** #2 Diesel (NEAT)

**Prep Date:** 11/5/2018

**Exp Date:** 11/5/2023

**Department:** dropr

**Vendor:** conoco

**Lot Number:**

**Balance ID:**

**Comments:** -18 Cloud peak. (Conoco Gas Sation 1240 S. 27th Billings, MT) 2nd Source

**Type:** Neat

**Prep By:** Ann Nebel

**Status:** New

**Final Volume:** 250 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
				11/5/2023
Stock Source	Base Units	Amount Added		



# Analytical RunID GCFID-HP5-B\_220111A Standards Traceability Report

**Standard ID:** DRO200430B  
**Standard Name:** O-Terphenyl  
**Prep Date:** 4/30/2020  
**Exp Date:** 9/30/2024  
**Department:** dropr  
**Vendor:** Chemservice  
**Lot Number:** 9972100  
**Balance ID:**  
**Comments:** ID#: 6271

**Type:** Neat  
**Prep By:** Ann Nebel  
**Status:** New

**Final Volume:** mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
o-Terphenyl	<a href="#">12650</a>	500	mg	9/30/2024
Stock Source	Base Units	Amount Added		



# Analytical RunID GCFID-HP5-B\_220111A Standards Traceability Report

**Standard ID:** DRO201014C

**Standard Name:** 1-Chlorooctadecane

**Prep Date:** 10/14/2019

**Exp Date:** 12/31/2024

**Department:** dropr

**Vendor:** CSI1

**Lot Number:** 10809500

**Balance ID:**

**Comments:** Date Certified: 12/9/16 ; N-10042-1G; 99.5% purity

**Type:** Neat

**Prep By:** Ann Nebel

**Status:** Open

**Final Volume:** mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
1-Chlorooctadecane	<a href="#">13192</a>	1	g	12/31/2024
Stock Source	Base Units	Amount Added		





# Analytical RunID GCFID-HP5-B\_220111A Standards Traceability Report

**Standard ID:** DRO201014D

**Standard Name:** n-Pentacosane

**Prep Date:** 10/14/2020

**Exp Date:** 2/28/2025

**Department:** dropr

**Vendor:** Chem Service

**Lot Number:** 9642200

**Balance ID:**

**Comments:** C-25; Used in AKDRO Marker

**Type:** Neat

**Prep By:** Ann Nebel

**Status:** New

**Final Volume:** mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
n-Pentacosane	<a href="#">13193</a>	100	mg	2/28/2025
Stock Source	Base Units	Amount Added		



# Analytical RunID GCFID-HP5-B\_220111A Standards Traceability Report

**Standard ID:** DRO211012B

**Standard Name:** #2 Diesel in Acetone 150,000 ug/mL

**Prep Date:** 10/12/2021

**Exp Date:** 11/5/2023

**Department:** dropr

**Vendor:**

**Lot Number:**

**Balance ID:** BAL-DRO

**Comments:** #2 Diesel in Acetone 150,000 ug/mL.

**Type:** Secondary

**Prep By:** Ann Nebel

**Status:** New

**Final Volume:** 25 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Acetone EA662	<a href="#">14050</a>	25	mL	11/5/2023

Stock Source	Base Units	Amount Added
DRO181105A	ug/mL	3.7507 g



# Analytical RunID GCFID-HP5-B\_220111A Standards Traceability Report

**Standard ID:** DRO211025B

**Standard Name:** Ali Hydro Std 1000ug/mL

**Prep Date:** 10/25/2021

**Exp Date:** 11/30/2024

**Department:** dropr

**Vendor:** Agilent

**Lot Number:** 0006643302

**Balance ID:**

**Comments:** Ali Hydro Std 1000ug/mL For CCVs.

**Type:** Primary

**Prep By:** Ann Nebel

**Status:** New

**Final Volume:** mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Aliphatic Hydrocarbon Standard	<a href="#">14434</a>	1	mL	11/30/2024
Stock Source	Base Units	Amount Added		



# Analytical RunID GCFID-HP5-B\_220111A Standards Traceability Report

**Spike ID:** DRO211101A  
**Spike Name:** OTP-4000 ug/mL DCM  
**Prep Date:** 11/1/2021  
**Exp Date:** 9/30/2024  
**Department:** dropr  
**Vendor:**  
**Lot Number:**  
**Balance ID:** BAL-DRO  
**Comments:** Used to Prep DRO-8015 ICAL and CCV Solutions

**Type:** Secondary  
**Prep By:** Ann Nebel  
**Status:** Open  
**Final Volume:** 25 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Dichloromethane EC328	<a href="#">14408</a>	25	mL	9/30/2024

Stock Source	Base Units	Amount Added
DRO200430B	ug/mL	0.1012 g



# Analytical RunID GCFID-HP5-B\_220111A Standards Traceability Report

**Standard ID:** DRO211214C

**Standard Name:** Diesel Fuel #2 50,000 ug/mL in DCM

**Prep Date:** 12/14/2021

**Exp Date:** 4/30/2023

**Department:** dropr

**Vendor:** Sigma-Aldrich

**Lot Number:** LRAC6316

**Balance ID:**

**Comments:** Diesel Fuel #2 For CCVs.

**Type:** Primary

**Prep By:** Ann Nebel

**Status:** New

**Final Volume:** mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Diesel Fuel No. 2	<a href="#">14623</a>	1	mL	4/30/2023

Stock Source	Base Units	Amount Added
DRO211214C	ug/mL	



# Analytical RunID GCFID-HP5-B\_220111A Standards Traceability Report

**Standard ID:** DRO211222B

**Standard Name:** EPH (4) SURR-1000 ug/mL ea. in Hexane

**Prep Date:** 12/22/2021

**Exp Date:** 5/31/2022

**Department:** dropr

**Vendor:**

**Lot Number:**

**Balance ID:** BAL-DRO

**Comments:** EPH (4) SURR-1000 ug/mL ea. in Hexane

**Type:** Secondary

**Prep By:** Jillian L Bostwick

**Status:** Open

**Final Volume:** 50 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Hexane EB754	<a href="#">14543</a>	50	mL	5/31/2022

Stock Source	Base Units	Amount Added
DRO180823A	ug/mL	0.0507 g
DRO200430B	ug/mL	0.0504 g
DRO180126C	ug/mL	0.0496 g
DRO201014C	ug/mL	0.0504 g



# Analytical RunID GCFID-HP5-B\_220111A Standards Traceability Report

**Standard ID:** DRO220102D

**Standard Name:** ALASKA MARKER-200ug/mL

**Prep Date:** 1/2/2022

**Exp Date:** 5/31/2022

**Department:** dropr

**Vendor:**

**Lot Number:**

**Balance ID:**

**Comments:** ALASKA MARKER w/ C-10, C-25, and OTP/COD. Optimal C-25 is 0.0012g.

**Type:** Secondary

**Prep By:** Ann Nebel

**Status:** New

**Final Volume:** 5.5 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Hexane EB754	<a href="#">14543</a>	3.3	mL	5/31/2022

Stock Source	Base Units	Amount Added
DRO201014D	ug/mL	0.0016 g
DRO211222B	ug/mL	1.1 mL
DRO211025B	ug/mL	1.1 mL

# Certificate of Analysis

Diesel Fuel No. 2

*Certified  
Reference  
Material*

## Description

Product ID UST148  
Lot LRAC6316  
Expiration Date April 2023  
Manufacturing Date April 2020  
Storage Conditions Room Temperature  
Solvent/Matrix DICHLOROMETHANE

ID #: 14623

Opened: \_\_\_\_\_

Diesel Fuel No. 2

Expires: 4/30/2023


Rec'd: 12/14/2021

Energy Laboratories Inc 1120 So. 27th Street  
Billings MT 59107

## Certified Values

Analyte	Certified Value <sup>1,4</sup>	Units	Raw Material Purity, %	Raw Material Lot	CAS
NO.2 FUEL OIL	50001 ± 2770	µg/mL	100.0	LA80505	68476-34-6

## Informational Values



## Additional Information:

Analytical Method Parameters:

Column: SPB-5, 30 m × 0.53 mm I.D., 1.5 µm film thickness (Column #214)

Carrier Gas: H<sub>2</sub>, Flow: 4.0 mL/min

Inlet Temperature: 250 °C, Injection Volume: 1.0 µL

Injection Mode: Split, Split Ratio: 10: 1

Temperature Program: 40 °C (Hold 2 min) @ 15 °C/min to 300 °C (Hold 5 min)

Detector: FID

Detector Temperature: 300 °C



**SIGMA-ALDRICH**

2931 Soldier Springs Rd. Laramie, Wyoming 82070 USA  
800-325-5832  
TechService@milliporesigma.com www.sigma-aldrich.com



# Description

Lot **LRAC6316**  
Expiration Date April 2023  
Manufacturing Date April 2020  
Storage Conditions Room Temperature  
Solvent/Matrix DICHLOROMETHANE

**1 Metrological traceability:** Traceable to the SI and higher order standards from NIST through an unbroken chain of comparisons. The balance used to weigh raw materials is accurate to +/-0.0001 g and calibrated regularly using mass standards traceable to NIST. All dilutions were performed gravimetrically. Additionally, individual analytes are traceable to NIST SRMs where available and specified above.  
**4 Ucrm - Uncertainty values** in this document are expressed as Expanded Uncertainty (Ucrm) corresponding to the 95% confidence interval. Ucrm is derived from the combined standard uncertainty multiplied by the coverage factor k, which is obtained from a t-distribution and degrees of freedom. The components of combined standard uncertainty include the uncertainties due to characterization, homogeneity, long term stability, and short term stability (transport). The components due to stability are generally considered to be negligible unless otherwise indicated by stability studies. The mathematical representation of the Ucrm calculation is as follows:

$$U_{CRM} = \sqrt{u_{char}^2 + u_{homogeneity}^2 + u_{stability}^2}$$

**k:** Coverage factor derived from a t-distribution table, based on the degrees of freedom of the data set. Assume 2.0 for a **Confidence interval = 95%**

**6 Analytical Value-** For QC verification of the certified value only- not to be used in calculations. Represents the analytical data obtained by comparison to a standard as analyzed by the method described in the CoA or another acceptable method. The result may differ from the certified value and UCRM based on method uncertainty as well as the uncertainty associated with the standard used for comparison.


**Traceability:** The standard was manufactured under an ISO/IEC 17025:2017 certified quality system. The balance used to weigh raw materials is accurate to +/- 0.0001g and calibrated regularly using mass standards traceable to NIST. All dilutions were performed gravimetrically. Additionally, individual analytes are traceable to NIST SRMs where available and specified above.

**Homogeneity:** Homogeneity was assessed in accordance with ISO 17034:2016. Completed units were sampled using a random stratified sampling protocol. The results of chemical analysis were then compared using a one-way analysis of variance approach as described by TNI EL-V3-2009 Appendix A.2. See Instructions for minimum sub-sample size.

Expiration is at end of month given on certificate and label.


MSDS reports for components comprising greater than 1.0% of the solution or 0.1% for components known to be carcinogens are available upon request.

**THIS PRODUCT WAS DESIGNED, PRODUCED AND VERIFIED FOR ACCURACY AND STABILITY IN ACCORDANCE WITH ISO/IEC 17025:2017 (ANAB Cert AT-1467) and ISO 17034:2016 (ANAB Cert AR-1470).**



Andy Ommen - QC Manager

Certification Date April 30, 2020  
Version 0-4302020



Mark Pooler - QA Supervisor



Anna

660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599  
1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729  
[info@chemservice.com](mailto:info@chemservice.com) • [www.chemservice.com](http://www.chemservice.com)

## CERTIFICATE OF ANALYSIS

### o-Terphenyl

CATALOG NUMBER N-12693-500MG  
LOT NUMBER 9972100  
DATE CERTIFIED 09/23/19  
EXPIRATION DATE 09/30/24  
CAS NUMBER 84-15-1  
MOLECULAR FORMULA C18H14  
MOLECULAR WEIGHT 230.32  
STORAGE Store in a cool dry place.  
HANDLING See Safety Data Sheet  
INTENDED USE For laboratory use only.

Analytical Test	Value
FT-IR SPECTROSCOPY	CONFORMS TO STRUCTURE
GC/MS SPECTRA ID	MATCHES NIST DATABASE
MELTING POINT (°C)	57.1
% PURITY (GC/FID)	99.5

Chem Service, Inc. guarantees the purity to be +/- 0.5% deviation prior to the expiration date shown on the label and exclusive of any customer contamination.

Certified By:

*Mary Beth O'Donnell*

Mary Beth O'Donnell  
CSM/TC

ID #: 12650

Opened: \_\_\_\_\_

o-Terphenyl

Expires: 9/30/2024


Rec'd: 4/30/2020

Energyl Laboratories Inc 1120 So. 27th Street  
Billings MT 59107

## CERTIFICATE OF ANALYSIS

### Analysis Method:

Catalog Number: N-12693-500MG  
Description: o-Terphenyl  
Lot Number: 9972100  
Expiration Date: 09/30/24



Chem Service is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015





## CERTIFICATE OF ANALYSIS

### Analysis Method:

Catalog Number: N-12693-500MG  
Description: o-Terphenyl  
Lot Number: 9972100  
Expiration Date: 09/30/24

Chem Service Inc      Area Percent Report

Data File: D:\msdchem\2019 DATA\0919\0923-01.D  
Acq On : 23 Sep 2019 10:40  
Operator :  
Sample : n-12693  
Misc :  
ALS Vial : 95

Integration Parameters: autoint1.e  
Integrator: ChemStation

DataAcq Meth: SCREEN.M  
Method : D:\msdchem\2019 DATA\0919\0903-09.D\ERIN.M

Signal : TIC: 0923-01.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	11.844	1597	1606	1613	BB	32038221	432253484	100.00%	100.000%

Sum of corrected areas: 432253484

ERIN.M Mon Sep 23 10:55:51 2019


660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599  
1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729  
[info@chemservice.com](mailto:info@chemservice.com) • [www.chemservice.com](http://www.chemservice.com)

## CERTIFICATE OF ANALYSIS

### Analysis Method:


Catalog Number: N-12693-500MG  
Description: o-Terphenyl  
Lot Number: 9972100  
Expiration Date: 09/30/24

Abundance

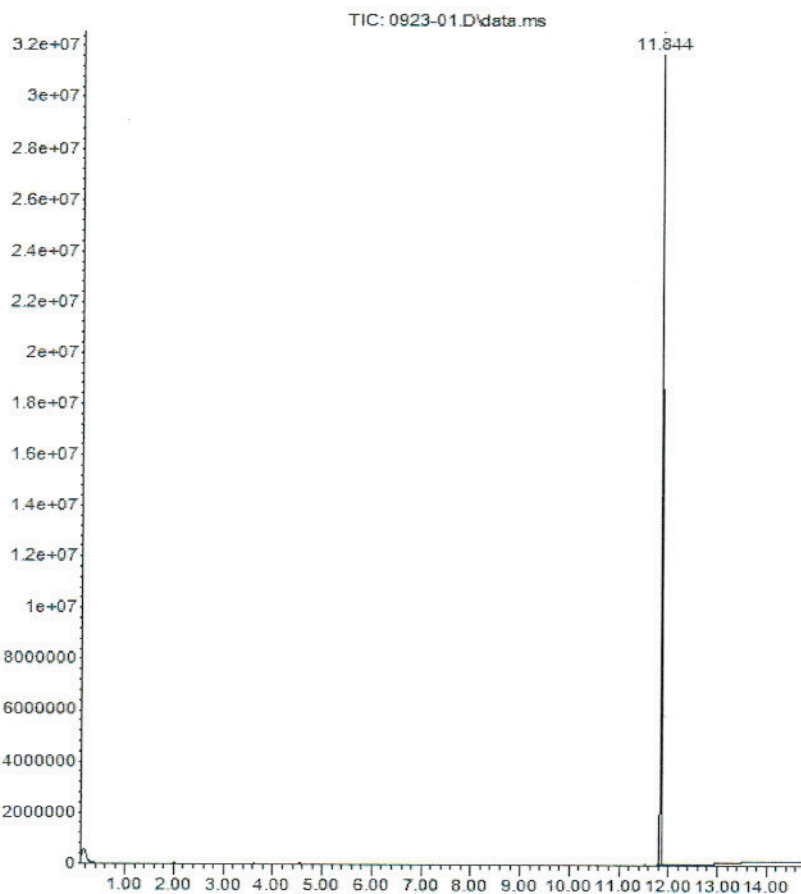

Time-->

Chem Service is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015




660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599  
1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729  
[info@chemservice.com](mailto:info@chemservice.com) • [www.chemservice.com](http://www.chemservice.com)

## CERTIFICATE OF ANALYSIS

### Analysis Method:

Catalog Number: N-12693-500MG  
Description: o-Terphenyl  
Lot Number: 9972100  
Expiration Date: 09/30/24

Abundance

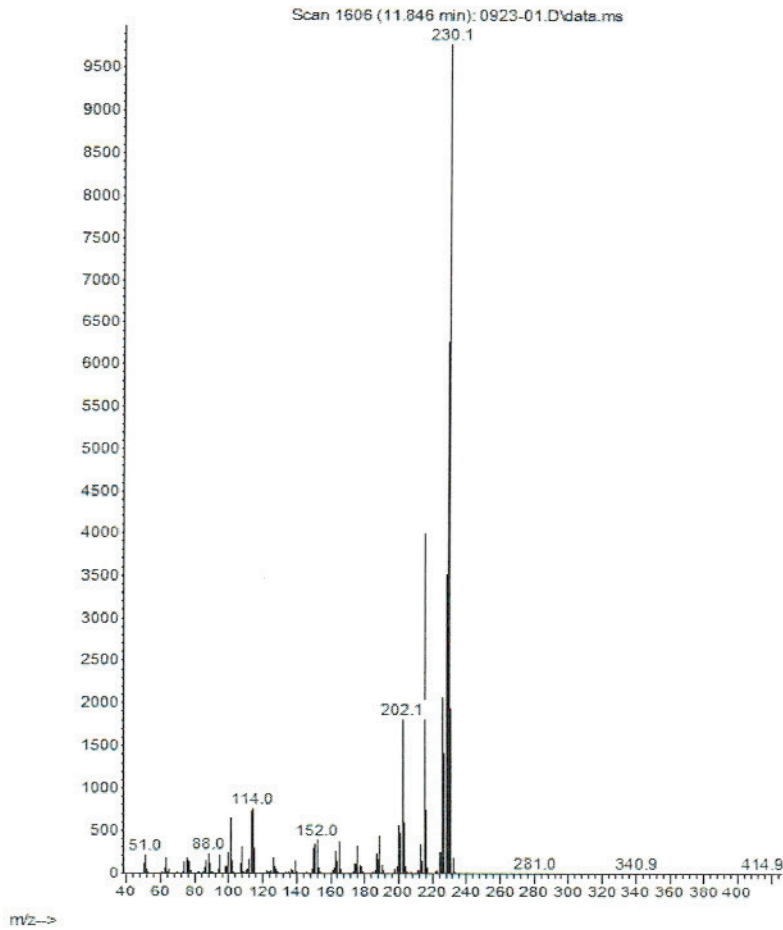

Chem Service is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015.



660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599  
1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729  
[info@chemservice.com](mailto:info@chemservice.com) • [www.chemservice.com](http://www.chemservice.com)

## CERTIFICATE OF ANALYSIS

### Analysis Method:

Catalog Number:	N-12693-500MG
Description:	o-Terphenyl
Lot Number:	9972100
Expiration Date:	09/30/24

Chem Service is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015




660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599  
 1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729  
[info@chemservice.com](mailto:info@chemservice.com) • [www.chemservice.com](http://www.chemservice.com)

Gas

Data file: C:\CHEM3\  
 Sample name: N-12893  
 Instrument: GC 2  
 Injection date: 8/23/2019 9:58:34 AM  
 Acq. method: SCREEN.M  
 Column name: HP-5

## CERTIFICATE OF ANALYSIS

Location: Vial 141  
 Injection volume: 1.0uL

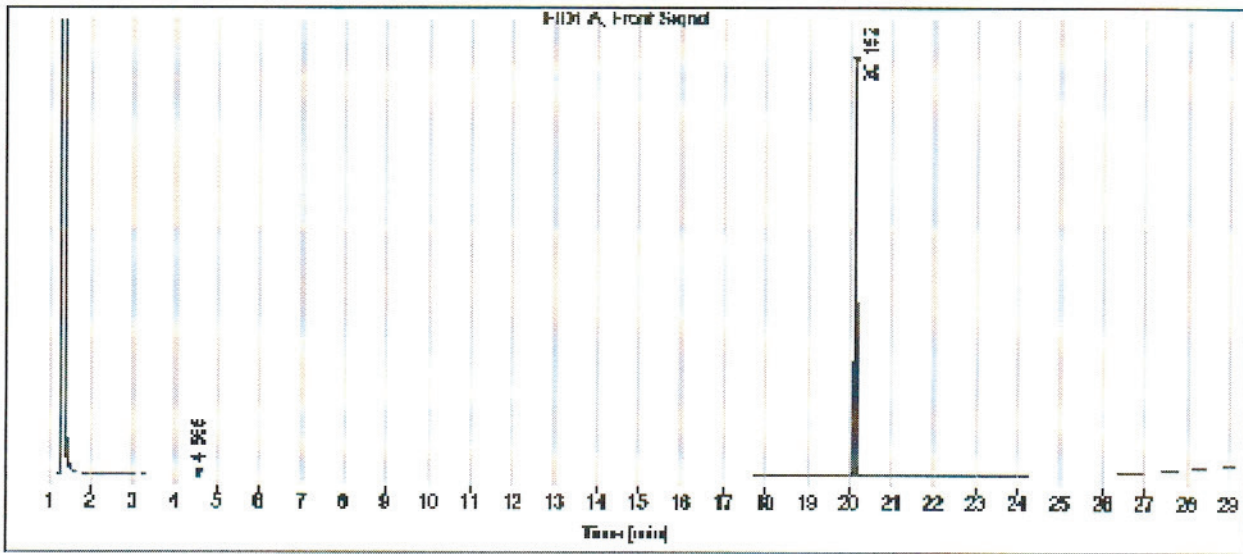

Signal: FID1 A, Front Signal

RT [min]	Type	Width [min]	Area	Height	Area%
4.565	BB	0.0305	1.2408	0.5122	0.11
20.152	BB	0.0391	1171.9556	439.4599	99.89
		Sum	1173.1963		

Chem Service is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015







# Analytical RunID GCFID-HP5-B\_220111c Standards Traceability Report

**Standard ID:** DRO210406A

**Standard Name:** Triacontane-d62 Surr For AK103 RRO

**Prep Date:** 4/6/2021

**Exp Date:** 4/6/2026

**Department:** dropr

**Vendor:** Sigma-Aldrich

**Lot Number:** MBBC4347

**Balance ID:**

**Comments:** Alaska surr [for AK103 RRO]

**Type:** Neat

**Prep By:** Ann Nebel

**Status:** New

**Final Volume:** mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Triacontane-d62-98 atom % D	<a href="#">13736</a>		mL	4/6/2026
Stock Source	Base Units	Amount Added		



# Analytical RunID GCFID-HP5-B\_220111c Standards Traceability Report

**Standard ID:** DRO210901A

**Standard Name:** 30W Motor Oil-Valvoline

**Prep Date:** 9/1/2021

**Exp Date:** 9/1/2026

**Department:** dropr

**Vendor:**

**Lot Number:** F1620C1

**Balance ID:**

**Comments:** Used to make 2nd Source Standard for AK103 method.

**Type:** Primary

**Prep By:** Jillian L Bostwick

**Status:** New

**Final Volume:** mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Valvoline SAE 30 Motor Oil	<a href="#">14232</a>		mL	9/1/2026
Stock Source	Base Units	Amount Added		



# Analytical RunID GCFID-HP5-B\_220111c Standards Traceability Report

**Standard ID:** DRO210901B

**Standard Name:** 40W Motor Oil-Valvoline

**Prep Date:** 9/1/2021

**Exp Date:** 9/1/2026

**Department:** dropr

**Vendor:**

**Lot Number:** L0717H2

**Balance ID:**

**Comments:** Used to Make 2nd Source Standards For Alaska AK103 RRO Method and Oil

**Type:** Primary

**Prep By:** Jillian L Bostwick

**Status:** New

**Final Volume:** mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Valvoline SAE 40 Motor Oil	<a href="#">14231</a>		mL	9/1/2026
Stock Source	Base Units	Amount Added		



# Analytical RunID GCFID-HP5-B\_220111c Standards Traceability Report

**Standard ID:** DRO210902A

**Standard Name:** 50,000 ug/mL Oil Std for RRO-In DCM

**Prep Date:** 9/2/2021

**Exp Date:** 9/1/2026

**Department:** dropr

**Vendor:**

**Lot Number:**

**Balance ID:** BAL-DRO

**Comments:** .625 g of 30W and 40 W each LCS for Oil range

**Type:** Secondary

**Prep By:** Jillian L Bostwick

**Status:** New

**Final Volume:** 25 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Dichloromethane EB867	<a href="#">14196</a>	25	mL	9/1/2026

Stock Source	Base Units	Amount Added
DRO210901A	ug/mL	0.6254 g
DRO210901B	ug/mL	0.6261 g



# Analytical RunID GCFID-HP5-B\_220111c Standards Traceability Report

**Standard ID:** DRO211006A

**Standard Name:** Triacontane SURR 2000 ug/mL

**Prep Date:** 10/6/2021

**Exp Date:** 4/6/2026

**Department:** dropr

**Vendor:**

**Lot Number:**

**Balance ID:** BAL-DRO

**Comments:** Triacontane SURR 2000 ug/mL

**Type:** Secondary

**Prep By:** Jillian L Bostwick

**Status:** New

**Final Volume:** 50 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Acetone DZ509	<a href="#">13553</a>	50	mL	4/6/2026

Stock Source	Base Units	Amount Added
DRO210406A	ug/mL	0.1001 g



# Analytical RunID GCFID-HP5-B\_220111c Standards Traceability Report

**Standard ID:** DRO211118A

**Standard Name:** 50,000 ug/mL Oil Std For AK103 RRO-In DCM

**Prep Date:** 11/18/2021

**Exp Date:** 10/31/2028

**Department:** dropr

**Vendor:** Restek

**Lot Number:** A0176667

**Balance ID:** Sartorius 4 place balance

**Comments:**

**Type:** Primary

**Prep By:** Ann Nebel

**Status:** Open

**Final Volume:** 1 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Residual Range Calibration Standard	<a href="#">14531</a>	1	mL	10/31/2028

Stock Source	Base Units	Amount Added
DRO211118A	ug/mL	



# CERTIFIED REFERENCE MATERIAL

110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

## Certificate of Analysis



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31817 **Lot No.:** A0176667

**Description :** Residual Range Calibration Standard (RCS)

Residual Range Calib Std (RCS) 50,000µg/mL, Methylene Chloride, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** October 31, 2028 **Storage:** 25°C nominal

**Ship:** Ambient

### CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)		
1	Motor Oil SAE30 & SAE40 Blend (Pennzoil) CAS # 64742-65-0.F Purity ----%	50,102.0 µg/mL	+/- 293.3582	µg/mL	Gravimetric
	(Lot A0126386)		+/- 1,492.1008	µg/mL	Unstressed
			+/- 1,591.3244	µg/mL	Stressed

**Solvent:** Methylene chloride  
CAS # 75-09-2  
Purity 99%

**ID #: 14531**

Opened: \_\_\_\_\_

Residual Range Calibration Standard

**Expires: 10/31/2028**

Rec'd: 11/18/2021

Energv Laboratories Inc 1120 So. 27th Street  
Billings MT 59107

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**


250°C

**Det. Temp:**

330°C

**Det. Type:**

FID



This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Sam Moodler*

Sam Moodler - Operations Tech I

Date Mixed: 22-Sep-2021

Balance: 1128360905

*Alexis Shelow*

Alexis Shelow - Operations Tech I

Date Passed: 23-Sep-2021

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value ( includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us) for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us).
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.

3050 Spruce Street, Saint Louis, MO 63103, USA

Website: [www.sigmaaldrich.com](http://www.sigmaaldrich.com)

Email USA: [techserv@sial.com](mailto:techserv@sial.com)

Outside USA: [eurtechserv@sial.com](mailto:eurtechserv@sial.com)

## Certificate of Analysis

Product Name:  
Triacontane-d62 - 98 atom % D

Product Number: 451789  
 Batch Number: MBBC4347  
 Brand: ALDRICH  
 CAS Number: 93952-07-9  
 MDL Number: MFCD00209794  
 Formula: C30D62  
 Formula Weight: 485.20 g/mol  
 Quality Release Date: 27 APR 2018



ID #: 13736

Opened: \_\_\_\_\_


Triacontane-d62-98 atom % D

Expires: 4/6/2026

Rec'd: 4/6/2021

Energx Laboratories Inc 1120 So. 27th Street  
 Billings MT 59107

Test	Specification	Result
Purity (HPLC)	≥ 99.0 %	99.0 %
Proton NMR Spectrum	Conforms to Structure	Conforms
D Enrichment	≥ 98.0 %	99.0 %
Initial Melting Point		60.0 °C
Final Melting Point		62.0 °C



Greg Abernathy, Supervisor  
 Quality Control  
 Miamisburg, Ohio US

Sigma-Aldrich warrants, that at the time of the quality release or subsequent retest date this product conformed to the information contained in this publication. The current Specification sheet may be available at Sigma-Aldrich.com. For further inquiries, please contact Technical Service. Purchaser must determine the suitability of the product for its particular use. See reverse side of invoice or packing slip for additional terms and conditions of sale.



## Prep Batch 163190 Standards Traceability Report

**Spike ID:** DRO181105A

**Spike Name:** #2 Diesel (NEAT)

**Prep Date:** 11/5/2018

**Exp Date:** 11/5/2023

**Department:** dropr

**Vendor:** conoco

**Lot Number:**

**Balance ID:**

**Comments:** -18 Cloud peak. (Conoco Gas Sation 1240 S. 27th Billings, MT) 2nd Source

**Type:** Neat

**Prep By:** Ann Nebel

**Status:** New

**Final Volume:** 250 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
				11/5/2023
Stock Source	Base Units	Amount Added		



## Prep Batch 163190 Standards Traceability Report

**Spike ID:** DRO200430B  
**Spike Name:** O-Terphenyl  
**Prep Date:** 4/30/2020  
**Exp Date:** 9/30/2024  
**Department:** dropr  
**Vendor:** Chemservice  
**Lot Number:** 9972100  
**Balance ID:**  
**Comments:** ID#: 6271

**Type:** Neat  
**Prep By:** Ann Nebel  
**Status:** New

**Final Volume:** mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
o-Terphenyl	<a href="#">12650</a>	500	mg	9/30/2024
Stock Source	Base Units	Amount Added		



## Prep Batch 163190 Standards Traceability Report

**Spike ID:** DRO210406A

**Spike Name:** Triacontane-d62 Surr For AK103 RRO

**Prep Date:** 4/6/2021

**Exp Date:** 4/6/2026

**Department:** dropr

**Vendor:** Sigma-Aldrich

**Lot Number:** MBBC4347

**Balance ID:**

**Comments:** Alaska surr [for AK103 RRO]

**Type:** Neat

**Prep By:** Ann Nebel

**Status:** New

**Final Volume:** mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Triacontane-d62-98 atom % D	<a href="#">13736</a>	500	mg	4/6/2026

Stock Source	Base Units	Amount Added
--------------	------------	--------------





## Prep Batch 163190 Standards Traceability Report

**Spike ID:** DRO210901A

**Spike Name:** 30W Motor Oil-Valvoline

**Prep Date:** 9/1/2021

**Exp Date:** 9/1/2026

**Department:** dropr

**Vendor:**

**Lot Number:** F1620C1

**Balance ID:**

**Comments:** Used to make 2nd Source Standard for AK103 method.

**Type:** Primary

**Prep By:** Jillian L Bostwick

**Status:** New

**Final Volume:** mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Valvoline SAE 30 Motor Oil	<a href="#">14232</a>		mL	9/1/2026
Stock Source	Base Units	Amount Added		



## Prep Batch 163190 Standards Traceability Report

**Spike ID:** DRO210901B

**Spike Name:** 40W Motor Oil-Valvoline

**Prep Date:** 9/1/2021

**Exp Date:** 9/1/2026

**Department:** dropr

**Vendor:**

**Lot Number:** L0717H2

**Balance ID:**

**Comments:** Used to Make 2nd Source Standards For Alaska AK103 RRO Method and Oil

**Type:** Primary

**Prep By:** Jillian L Bostwick

**Status:** New

**Final Volume:** mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Valvoline SAE 40 Motor Oil	<a href="#">14231</a>		mL	9/1/2026
Stock Source	Base Units	Amount Added		



## Prep Batch 163190 Standards Traceability Report

**Spike ID:** DRO210902A

**Spike Name:** 50,000 ug/mL Oil Std for RRO-In DCM

**Prep Date:** 9/2/2021

**Exp Date:** 9/1/2026

**Department:** dropr

**Vendor:**

**Lot Number:**

**Balance ID:** BAL-DRO

**Comments:** .625 g of 30W and 40 W each LCS for Oil range

**Type:** Secondary

**Prep By:** Jillian L Bostwick

**Status:** New

**Final Volume:** 25 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Dichloromethane EB867	<a href="#">14196</a>	25	mL	9/1/2026

Stock Source	Base Units	Amount Added
DRO210901A	ug/mL	0.6254 g
DRO210901B	ug/mL	0.6261 g





## Prep Batch 163190 Standards Traceability Report

**Spike ID:** DRO210902B

**Spike Name:** 30,000 ug/mL Oil Std For RRO-In DCM

**Prep Date:** 9/2/2021

**Exp Date:** 9/1/2026

**Department:** dropr

**Vendor:**

**Lot Number:**

**Balance ID:** BAL-DRO

**Comments:**

**Type:** Secondary

**Prep By:** Jillian L Bostwick

**Status:** New

**Final Volume:** 4 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Dichloromethane EB867	<a href="#">14196</a>	1.6	mL	9/1/2026

Stock Source	Base Units	Amount Added
DRO210902A	ug/mL	2.4 mL



## Prep Batch 163190 Standards Traceability Report

**Spike ID:** DRO210902C

**Spike Name:** 3,000 ug/mL Oil Std For MDLS-In DCM

**Prep Date:** 9/2/2021

**Exp Date:** 9/1/2026

**Department:** dropr

**Vendor:**

**Lot Number:**

**Balance ID:** BAL-DRO

**Comments:** 100 uL for MDL = .3 mg/L

**Type:** Secondary

**Prep By:** Jillian L Bostwick

**Status:** New

**Final Volume:** 4 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Dichloromethane EB867	<a href="#">14196</a>	3.6	mL	9/1/2026

Stock Source	Base Units	Amount Added
DRO210902B	ug/mL	0.4 mL



## Prep Batch 163190 Standards Traceability Report

**Spike ID:** DRO211006A

**Spike Name:** Triacontane SURR 2000 ug/mL

**Prep Date:** 10/6/2021

**Exp Date:** 4/6/2026

**Department:** dropr

**Vendor:**

**Lot Number:**

**Balance ID:** BAL-DRO

**Comments:** Triacontane SURR 2000 ug/mL

**Type:** Primary

**Prep By:** Jillian L Bostwick

**Status:** New

**Final Volume:** 50 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Acetone DZ509	<a href="#">13553</a>	50	mL	4/6/2026

Stock Source	Base Units	Amount Added
DRO210406A	ug/mL	0.1001 g



## Prep Batch 163190 Standards Traceability Report

**Spike ID:** DRO211006B

**Spike Name:** Triacontane SURR 20 ug/mL

**Prep Date:** 10/6/2021

**Exp Date:** 4/6/2026

**Department:** dropr

**Vendor:**

**Lot Number:**

**Balance ID:** BAL-DRO

**Comments:** 100X dilution of Triacontane SURR 2000 ug/mL

**Type:** Secondary

**Prep By:** Jillian L Bostwick

**Status:** New

**Final Volume:** 4 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Acetone DZ509	<a href="#">13553</a>	3.96	mL	4/6/2026

Stock Source	Base Units	Amount Added
DRO211006A	ug/mL	40 uL



## Prep Batch 163190 Standards Traceability Report

**Spike ID:** DRO211213A

**Spike Name:** OTP only SURR 2000 ug/mL

**Prep Date:** 12/13/2021

**Exp Date:** 9/30/2024

**Department:** dropr

**Vendor:**

**Lot Number:**

**Balance ID:** BAL-DRO

**Comments:** OTP SURR 2000 ug/mL

**Type:** Primary

**Prep By:** Jillian L Bostwick

**Status:** New

**Final Volume:** 100 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Acetone DZ509	<a href="#">13553</a>	100	mL	9/30/2024

Stock Source	Base Units	Amount Added
DRO200430B	ug/mL	0.2015 g



## Prep Batch 163190 Standards Traceability Report

**Spike ID:** DRO220106C

**Spike Name:** #2 Diesel in Acetone 150,000 ug/mL

**Prep Date:** 1/6/2022

**Exp Date:** 11/5/2023

**Department:** dropr

**Vendor:**

**Lot Number:**

**Balance ID:** BAL-DRO

**Comments:**

**Type:** Secondary

**Prep By:** Ann Nebel

**Status:** New

**Final Volume:** 25 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Acetone DZ509	<a href="#">13553</a>	25	mL	11/5/2023
Stock Source	Base Units	Amount Added		
DRO181105A	ug/mL	3.7506 g		



## Prep Batch 163190 Standards Traceability Report

**Spike ID:** DRO220112A

**Spike Name:** 50,000 ug/mL Oil Std for RRO-In DCM

**Prep Date:** 1/12/2022

**Exp Date:** 9/1/2026

**Department:** dropr

**Vendor:**

**Lot Number:**

**Balance ID:** BAL-DRO

**Comments:** .625 g of 30W and 40 W each LCS for Oil range

**Type:** Secondary

**Prep By:** Jillian L Bostwick

**Status:** New

**Final Volume:** 25 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Dichloromethane EC832	<a href="#">14647</a>	25	mL	9/1/2026

Stock Source	Base Units	Amount Added
DRO210901A	ug/mL	0.6225 g
DRO210901B	ug/mL	0.6273 g



## Prep Batch 163190 Standards Traceability Report

**Spike ID:** DRO220119A

**Spike Name:** Triacontane SURR 1000 ug/mL

**Prep Date:** 1/19/2022

**Exp Date:** 4/6/2026

**Department:** dropr

**Vendor:**

**Lot Number:**

**Balance ID:** BAL-DRO

**Comments:** 2X dilution of Triacontane SURR 2000 ug/mL

**Type:** Secondary

**Prep By:** Jillian L Bostwick

**Status:** New

**Final Volume:** 10 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Dichloromethane EC849	<a href="#">14747</a>	5	mL	4/6/2026

Stock Source	Base Units	Amount Added
DRO211006A	ug/mL	5 mL



660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599  
1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729  
[info@chemservice.com](mailto:info@chemservice.com) • [www.chemservice.com](http://www.chemservice.com)

## CERTIFICATE OF ANALYSIS

### o-Terphenyl

CATALOG NUMBER N-12693-500MG  
LOT NUMBER 9972100  
DATE CERTIFIED 09/23/19  
EXPIRATION DATE 09/30/24  
CAS NUMBER 84-15-1  
MOLECULAR FORMULA C18H14  
MOLECULAR WEIGHT 230.32  
STORAGE Store in a cool dry place.  
HANDLING See Safety Data Sheet  
INTENDED USE For laboratory use only.

Analytical Test	Value
FT-IR SPECTROSCOPY	CONFORMS TO STRUCTURE
GC/MS SPECTRA ID	MATCHES NIST DATABASE
MELTING POINT (°C)	57.1
% PURITY (GC/FID)	99.5

Chem Service, Inc. guarantees the purity to be +/- 0.5% deviation prior to the expiration date shown on the label and exclusive of any customer contamination.

Certified By:

*Mary Beth O'Donnell*

Mary Beth O'Donnell  
CSM/TC

ID #: 12650

Opened: \_\_\_\_\_

o-Terphenyl

Expires: 9/30/2024

Rec'd: 4/30/2020

Energyl Laboratories Inc 1120 So. 27th Street  
Billings MT 59107


Chem Service is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015



## CERTIFICATE OF ANALYSIS

### Analysis Method:

Catalog Number: N-12693-500MG  
Description: o-Terphenyl  
Lot Number: 9972100  
Expiration Date: 09/30/24



Chem Service is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015



## CERTIFICATE OF ANALYSIS

### Analysis Method:

Catalog Number: N-12693-500MG  
Description: o-Terphenyl  
Lot Number: 9972100  
Expiration Date: 09/30/24

Chem Service Inc      Area Percent Report

Data File: D:\msdchem\2019 DATA\0919\0923-01.D  
Acq On : 23 Sep 2019 10:40  
Operator :  
Sample : n-12693  
Misc :  
ALS Vial : 95

Integration Parameters: autoint1.e  
Integrator: ChemStation

DataAcq Meth: SCREEN.M  
Method : D:\msdchem\2019 DATA\0919\0903-09.D\ERIN.M

Signal : TIC: 0923-01.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	11.844	1597	1606	1613	BB	32038221	432253484	100.00%	100.000%

Sum of corrected areas: 432253484

ERIN.M Mon Sep 23 10:55:51 2019


660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599  
1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729  
[info@chemservice.com](mailto:info@chemservice.com) • [www.chemservice.com](http://www.chemservice.com)

## CERTIFICATE OF ANALYSIS

### Analysis Method:

Catalog Number: N-12693-500MG  
Description: o-Terphenyl  
Lot Number: 9972100  
Expiration Date: 09/30/24

Abundance

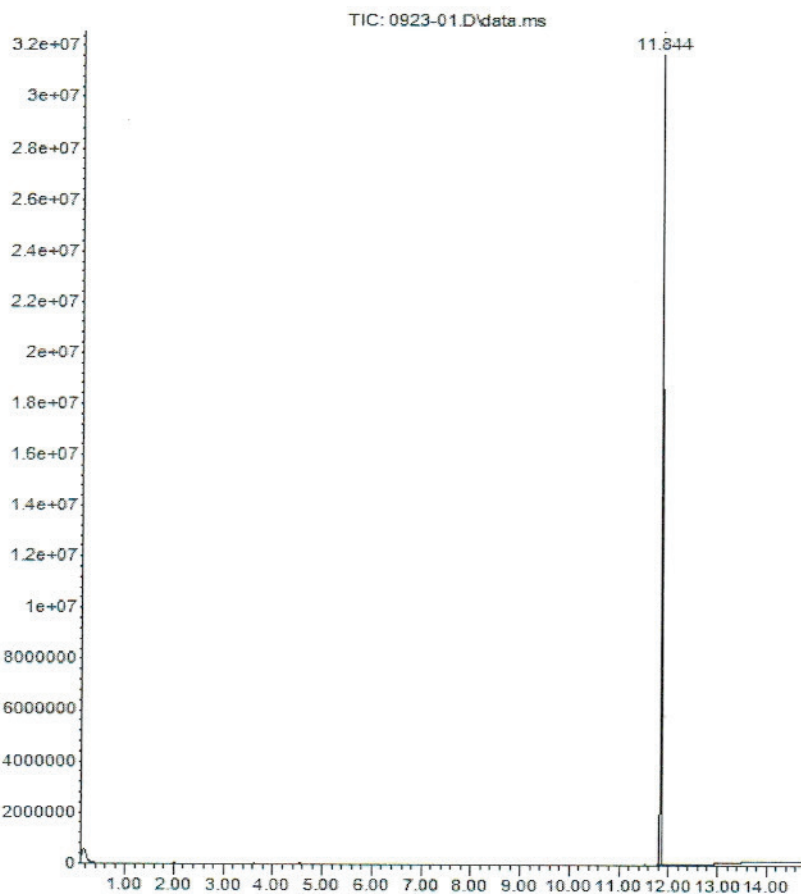

Chem Service is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015






660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599  
1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729  
[info@chemservice.com](mailto:info@chemservice.com) • [www.chemservice.com](http://www.chemservice.com)

## CERTIFICATE OF ANALYSIS

### Analysis Method:

Catalog Number: N-12693-500MG  
Description: o-Terphenyl  
Lot Number: 9972100  
Expiration Date: 09/30/24

Abundance

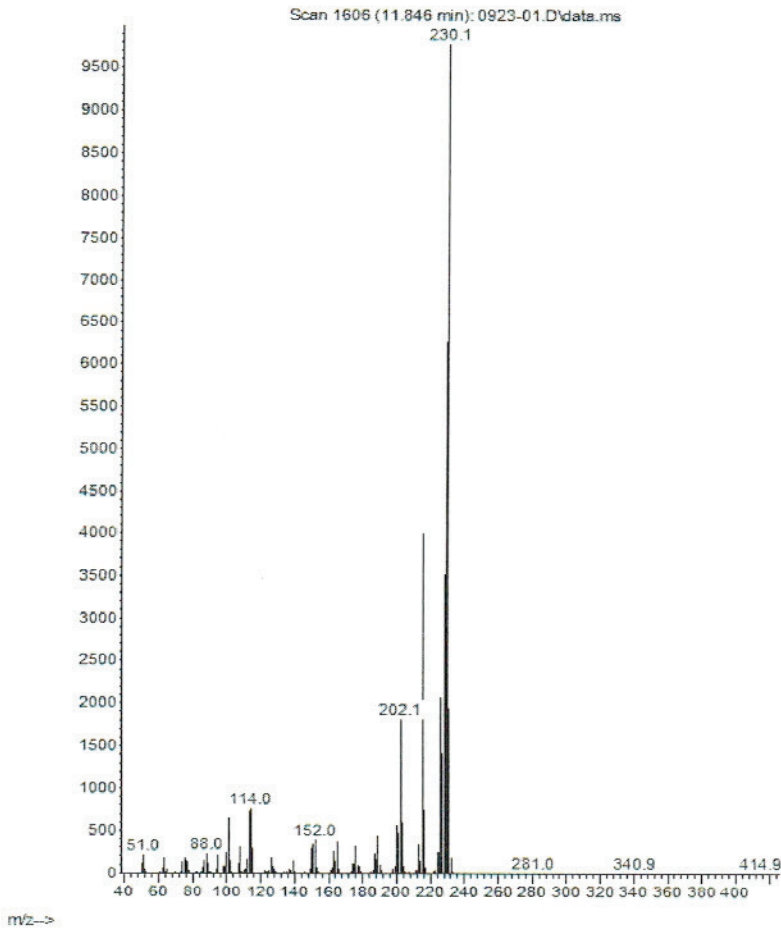

Chem Service is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015.



660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599  
1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729  
[info@chemservice.com](mailto:info@chemservice.com) • [www.chemservice.com](http://www.chemservice.com)

## CERTIFICATE OF ANALYSIS

### Analysis Method:

Catalog Number:	N-12693-500MG
Description:	o-Terphenyl
Lot Number:	9972100
Expiration Date:	09/30/24

Chem Service is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015




660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599  
 1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729  
[info@chemservice.com](mailto:info@chemservice.com) • [www.chemservice.com](http://www.chemservice.com)

Gas

Data file: C:\CHEM3\  
 Sample name: N-12893  
 Instrument: GC 2  
 Injection date: 8/23/2019 9:58:34 AM  
 Acq. method: SCREEN.M  
 Column name: HP-5

## CERTIFICATE OF ANALYSIS

Location: Vial 141  
 Injection volume: 1.0uL

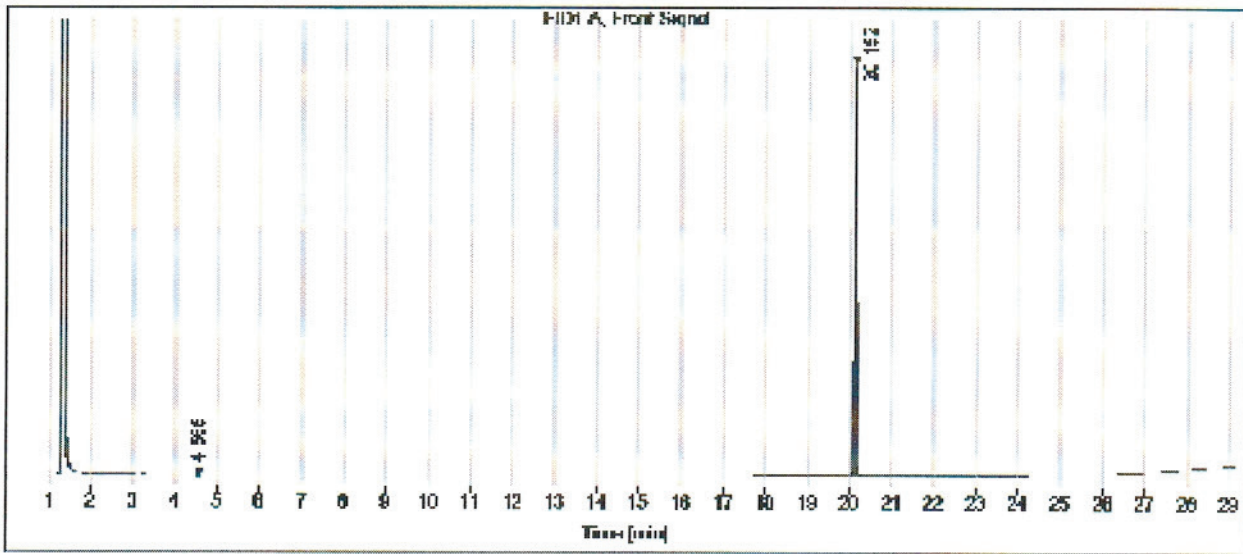

Signal: FID1 A, Front Signal

RT [min]	Type	Width [min]	Area	Height	Area%
4.565	BB	0.0305	1.2408	0.5122	0.11
20.152	BB	0.0391	1171.9556	439.4599	99.89
	Sum		1173.1963		

Chem Service is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015



3050 Spruce Street, Saint Louis, MO 63103, USA  
 Website: www.sigmaaldrich.com  
 Email USA: techserv@sial.com  
 Outside USA: eurtechserv@sial.com

## Certificate of Analysis

Product Name:  
 Triacontane-d62 - 98 atom % D

Product Number: 451789  
 Batch Number: MBBC4347  
 Brand: ALDRICH  
 CAS Number: 93952-07-9  
 MDL Number: MFCD00209794  
 Formula: C30D62  
 Formula Weight: 485.20 g/mol  
 Quality Release Date: 27 APR 2018



ID #: 13736

Opened: \_\_\_\_\_


Triacontane-d62-98 atom % D

Expires: 4/6/2026

Rec'd: 4/6/2021

Energx Laboratories Inc 1120 So. 27th Street  
 Billings MT 59107

Test	Specification	Result
Purity (HPLC)	≥ 99.0 %	99.0 %
Proton NMR Spectrum	Conforms to Structure	Conforms
D Enrichment	≥ 98.0 %	99.0 %
Initial Melting Point		60.0 °C
Final Melting Point		62.0 °C



Greg Abernathy, Supervisor  
 Quality Control  
 Miamisburg, Ohio US

Sigma-Aldrich warrants, that at the time of the quality release or subsequent retest date this product conformed to the information contained in this publication. The current Specification sheet may be available at Sigma-Aldrich.com. For further inquiries, please contact Technical Service. Purchaser must determine the suitability of the product for its particular use. See reverse side of invoice or packing slip for additional terms and conditions of sale.





# Analytical RunID GCFID-HP5-B\_220124C Standards Traceability Report

**Standard ID:** DRO200430B

**Standard Name:** O-Terphenyl

**Prep Date:** 4/30/2020

**Exp Date:** 9/30/2024

**Department:** dropr

**Vendor:** Chemservice

**Lot Number:** 9972100

**Balance ID:**

**Comments:** ID#: 6271

**Type:** Neat

**Prep By:** Ann Nebel

**Status:** New

**Final Volume:** mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
o-Terphenyl	<a href="#">12650</a>	500	mg	9/30/2024
Stock Source	Base Units	Amount Added		



# Analytical RunID GCFID-HP5-B\_220124C Standards Traceability Report

**Standard ID:** DRO210406A

**Standard Name:** Triacontane-d62 Surr For AK103 RRO

**Prep Date:** 4/6/2021

**Exp Date:** 4/6/2026

**Department:** dropr

**Vendor:** Sigma-Aldrich

**Lot Number:** MBBC4347

**Balance ID:**

**Comments:** Alaska surr [for AK103 RRO]

**Type:** Neat

**Prep By:** Ann Nebel

**Status:** New

**Final Volume:** mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Triacontane-d62-98 atom % D	<a href="#">13736</a>	500	mg	4/6/2026
Stock Source	Base Units	Amount Added		



# Analytical RunID GCFID-HP5-B\_220124C Standards Traceability Report

**Standard ID:** DRO211006A

**Standard Name:** Triacontane SURR 2000 ug/mL

**Prep Date:** 10/6/2021

**Exp Date:** 4/6/2026

**Department:** dropr

**Vendor:**

**Lot Number:**

**Balance ID:** BAL-DRO

**Comments:** Triacontane SURR 2000 ug/mL

**Type:** Primary

**Prep By:** Jillian L Bostwick

**Status:** New

**Final Volume:** 50 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Acetone DZ509	<a href="#">13553</a>	50	mL	4/6/2026

Stock Source	Base Units	Amount Added
DRO210406A	ug/mL	0.1001 g



# Analytical RunID GCFID-HP5-B\_220124C Standards Traceability Report

**Spike ID:** DRO211101A

**Spike Name:** OTP-4000 ug/mL DCM

**Prep Date:** 11/1/2021

**Exp Date:** 9/30/2024

**Department:** dropr

**Vendor:**

**Lot Number:**

**Balance ID:** BAL-DRO

**Comments:** Used to Prep DRO-8015 ICAL and CCV Solutions

**Type:** Secondary

**Prep By:** Ann Nebel

**Status:** Open

**Final Volume:** 25 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Dichloromethane EC328	<a href="#">14408</a>	25	mL	9/30/2024

Stock Source	Base Units	Amount Added
DRO200430B	ug/mL	0.1012 g



# Analytical RunID GCFID-HP5-B\_220124C Standards Traceability Report

**Standard ID:** DRO211118A

**Standard Name:** 50,000 ug/mL Oil Std For AK103 RRO-In DCM

**Prep Date:** 11/18/2021

**Exp Date:** 10/31/2028

**Department:** dropr

**Vendor:** Restek

**Lot Number:** A0176667

**Balance ID:** Sartorius 4 place balance

**Comments:**

**Type:** Primary

**Prep By:** Ann Nebel

**Status:** Open

**Final Volume:** 1 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Residual Range Calibration Standard	<a href="#">14531</a>	1	mL	10/31/2028
Stock Source	Base Units	Amount Added		
DRO211118A	ug/mL			



# Analytical RunID GCFID-HP5-B\_220124C Standards Traceability Report

**Standard ID:** DRO211214C

**Standard Name:** Diesel Fuel #2 50,000 ug/mL in DCM

**Prep Date:** 12/14/2021

**Exp Date:** 4/30/2023

**Department:** dropr

**Vendor:** Sigma-Aldrich

**Lot Number:** LRAC6316

**Balance ID:**

**Comments:** Diesel Fuel #2 For CCVs.

**Type:** Primary

**Prep By:** Ann Nebel

**Status:** New

**Final Volume:** mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Diesel Fuel No. 2	<a href="#">14623</a>	1	mL	4/30/2023

Stock Source	Base Units	Amount Added
DRO211214C	ug/mL	



# Analytical RunID GCFID-HP5-B\_220124C Standards Traceability Report

**Standard ID:** DRO220106B

**Standard Name:** Triacontane SURR 1000 ug/mL

**Prep Date:** 1/6/2022

**Exp Date:** 4/6/2026

**Department:** dropr

**Vendor:**

**Lot Number:**

**Balance ID:** BAL-DRO

**Comments:** 2X dilution of Triacontane SURR 2000 ug/mL

**Type:** Secondary

**Prep By:** Jillian L Bostwick

**Status:** New

**Final Volume:** 10 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Dichloromethane EC832	<a href="#">14647</a>	5	mL	4/6/2026
Stock Source	Base Units	Amount Added		
DRO211006A	ug/mL	5 mL		



# Analytical RunID GCFID-HP5-B\_220124C Standards Traceability Report

**Standard ID:** DRO220110A

**Standard Name:** Carbon Scan STD-Marker

**Prep Date:** 1/11/2022

**Exp Date:** 7/13/2026

**Department:** dropr

**Vendor:** ASI2

**Lot Number:** 55064

**Balance ID:**

**Comments:** FOR Qualitative analyst only.31 compounds-C5 to C30,32,34,36,38,40.

**Type:** Neat

**Prep By:** Ann Nebel

**Status:** Open

**Final Volume:** 1.2 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
n-Hydrocarbons- C5 to C30, C32, C34, C36, C38, C40	<a href="#">14737</a>	1.2	mL	7/13/2026

Stock Source	Base Units	Amount Added
DRO220110A	ug/mL	





# Analytical RunID GCFID-HP5-B\_220124C Standards Traceability Report

**Standard ID:** DRO220111A

**Standard Name:** Carbon Scan STD-Marker

**Prep Date:** 1/11/2022

**Exp Date:** 7/13/2026

**Department:** dropr

**Vendor:** ASI2

**Lot Number:** 071306

**Balance ID:**

**Comments:** FOR Qualitative analyst only.31 compounds-C5 to C30,32,34,36,38,40.

**Type:** Primary

**Prep By:** Ann Nebel

**Status:** Open

**Final Volume:** 2.4 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Carbon Disulfide 55064	<a href="#">7477</a>	1.2	mL	7/13/2026

Stock Source	Base Units	Amount Added
DRO220110A	ug/mL	1.2 mL



# Analytical RunID GCFID-HP5-B\_220124C Standards Traceability Report

**Standard ID:** DRO220118A

**Standard Name:** 5,000 ug/mL RRO CCV 200 ug/mL Triacontane

**Type:** Secondary

**Prep Date:** 1/18/2022

**Prep By:** Ann Nebel

**Exp Date:** 4/6/2026

**Status:** New

**Department:** dropr

**Vendor:**

**Final Volume:** 4 mL

**Lot Number:**

**Balance ID:**

**Comments:** CCV for AK102 and 8015C RRO.

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Dichloromethane EC849	<a href="#">14747</a>	2.8	mL	4/6/2026

Stock Source	Base Units	Amount Added
DRO220106B	ug/mL	800 µL
DRO211118A	ug/mL	400 µL



# Analytical RunID GCFID-HP5-B\_220124C Standards Traceability Report

**Standard ID:** DRO220124A

**Standard Name:** 8015 CCV-15,000ug/mL + 200 OTP

**Prep Date:** 1/24/2022

**Exp Date:** 4/30/2023

**Department:** dropr

**Vendor:**

**Lot Number:**

**Balance ID:**

**Comments:** 8015DRO CCV MIX-15,000ug/mL +200 OTP #2 Diesel

**Type:** Secondary

**Prep By:** Jillian L Bostwick

**Status:** New

**Final Volume:** 4 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Dichloromethane EC849	<a href="#">14747</a>	2.6	mL	4/30/2023

Stock Source	Base Units	Amount Added
DRO211214C	ug/mL	1.2 mL
DRO211101A	ug/mL	0.2 mL

660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599  
1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729  
[info@chemservice.com](mailto:info@chemservice.com) • [www.chemservice.com](http://www.chemservice.com)

## CERTIFICATE OF ANALYSIS

### o-Terphenyl

CATALOG NUMBER N-12693-500MG  
LOT NUMBER 9972100  
DATE CERTIFIED 09/23/19  
EXPIRATION DATE 09/30/24  
CAS NUMBER 84-15-1  
MOLECULAR FORMULA C18H14  
MOLECULAR WEIGHT 230.32  
STORAGE Store in a cool dry place.  
HANDLING See Safety Data Sheet  
INTENDED USE For laboratory use only.

Analytical Test	Value
FT-IR SPECTROSCOPY	CONFORMS TO STRUCTURE
GC/MS SPECTRA ID	MATCHES NIST DATABASE
MELTING POINT (°C)	57.1
% PURITY (GC/FID)	99.5

Chem Service, Inc. guarantees the purity to be +/- 0.5% deviation prior to the expiration date shown on the label and exclusive of any customer contamination.

Certified By:

*Mary Beth O'Donnell*

Mary Beth O'Donnell  
CSM/TC

ID #: 12650

Opened: \_\_\_\_\_

o-Terphenyl

Expires: 9/30/2024

Rec'd: 4/30/2020

Energyl Laboratories Inc 1120 So. 27th Street  
Billings MT 59107


Chem Service is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015



## CERTIFICATE OF ANALYSIS

### Analysis Method:

Catalog Number: N-12693-500MG  
Description: o-Terphenyl  
Lot Number: 9972100  
Expiration Date: 09/30/24

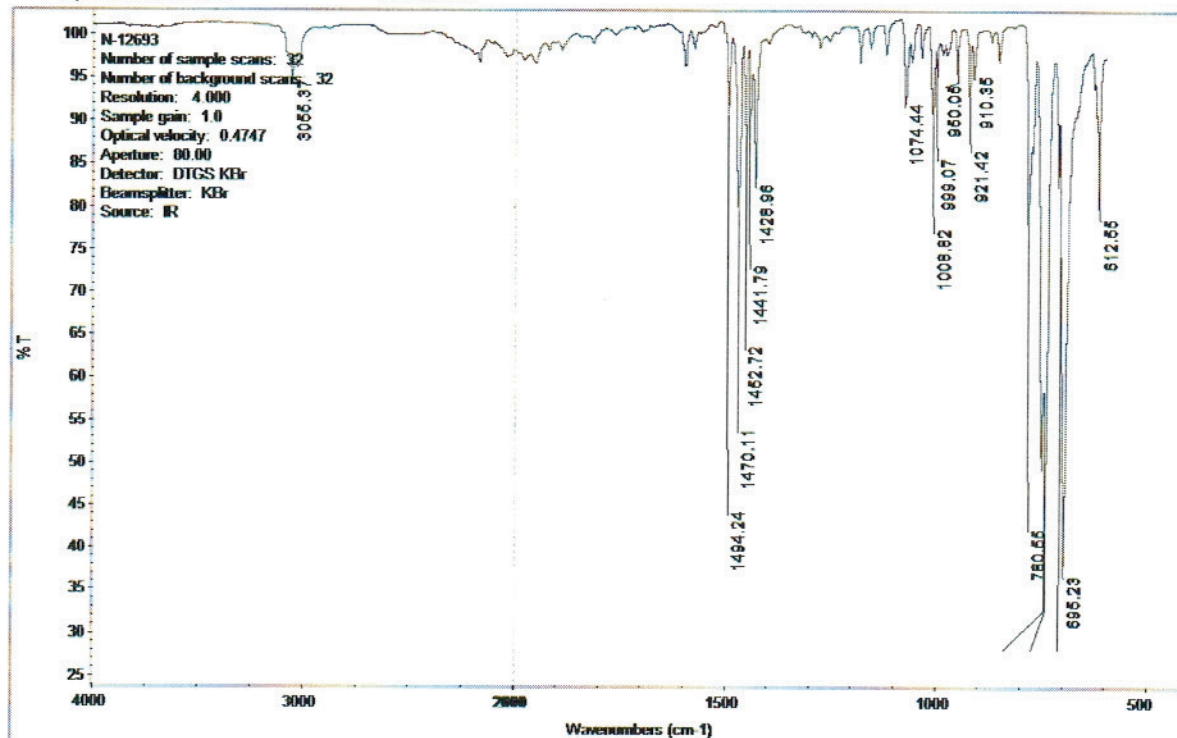

Chem Service is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015



660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599  
1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729  
[info@chemservice.com](mailto:info@chemservice.com) • [www.chemservice.com](http://www.chemservice.com)

## CERTIFICATE OF ANALYSIS

### Analysis Method:

Catalog Number: N-12693-500MG  
Description: o-Terphenyl  
Lot Number: 9972100  
Expiration Date: 09/30/24

Chem Service Inc      Area Percent Report

Data File: D:\msdchem\2019 DATA\0919\0923-01.D  
Acq On : 23 Sep 2019 10:40  
Operator :  
Sample : n-12693  
Misc :  
ALS Vial : 95

Integration Parameters: autoint1.e  
Integrator: ChemStation

DataAcq Meth: SCREEN.M  
Method : D:\msdchem\2019 DATA\0919\0903-09.D\ERIN.M

Signal : TIC: 0923-01.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	11.844	1597	1606	1613	BB	32038221	432253484	100.00%	100.000%

Sum of corrected areas: 432253484

ERIN.M Mon Sep 23 10:55:51 2019

Chem Service is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015






## CERTIFICATE OF ANALYSIS

### Analysis Method:

Catalog Number: N-12693-500MG  
Description: o-Terphenyl  
Lot Number: 9972100  
Expiration Date: 09/30/24

Abundance

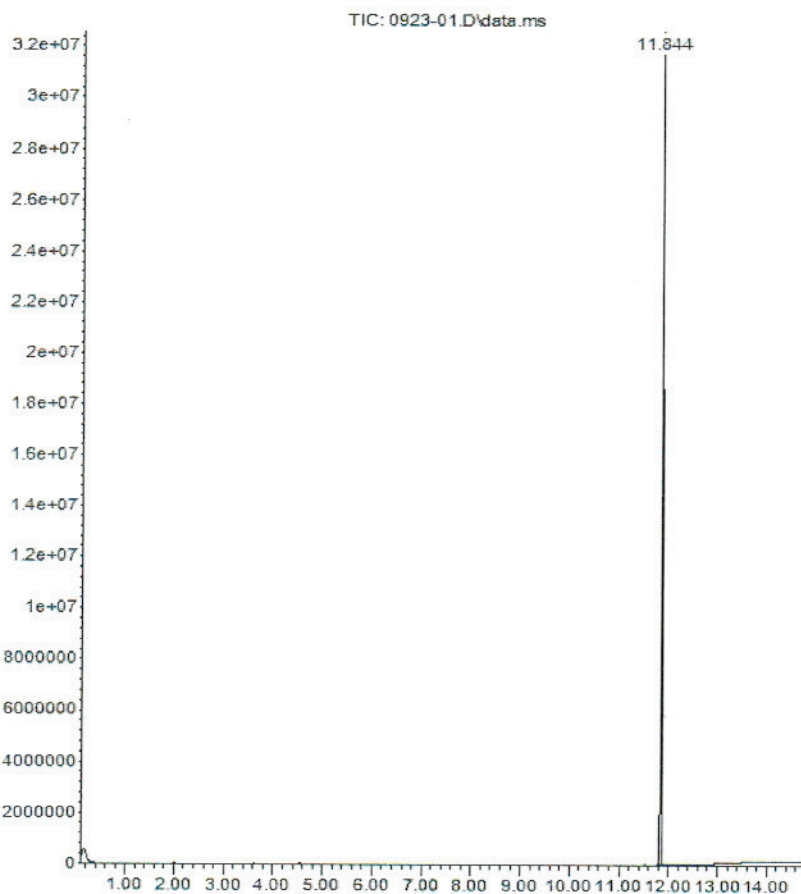

Chem Service is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015




660 Tower Lane • P. O. Box 599 • West Chester, PA 19381-0599  
1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729  
[info@chemservice.com](mailto:info@chemservice.com) • [www.chemservice.com](http://www.chemservice.com)

## CERTIFICATE OF ANALYSIS

### Analysis Method:

Catalog Number: N-12693-500MG  
Description: o-Terphenyl  
Lot Number: 9972100  
Expiration Date: 09/30/24

Abundance



Chem Service is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015.





660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599  
1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729  
[info@chemservice.com](mailto:info@chemservice.com) • [www.chemservice.com](http://www.chemservice.com)

## CERTIFICATE OF ANALYSIS

### Analysis Method:

Catalog Number:	N-12693-500MG
Description:	o-Terphenyl
Lot Number:	9972100
Expiration Date:	09/30/24

Chem Service is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015




660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599  
 1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729  
[info@chemservice.com](mailto:info@chemservice.com) • [www.chemservice.com](http://www.chemservice.com)

Gas

Data file: C:\CHEM3\  
 Sample name: N-12893  
 Instrument: GC 2  
 Injection date: 8/23/2019 9:58:34 AM  
 Acq. method: SCREEN.M  
 Column name: HP-5

## CERTIFICATE OF ANALYSIS

Location: Vial 141  
 Injection volume: 1.0uL

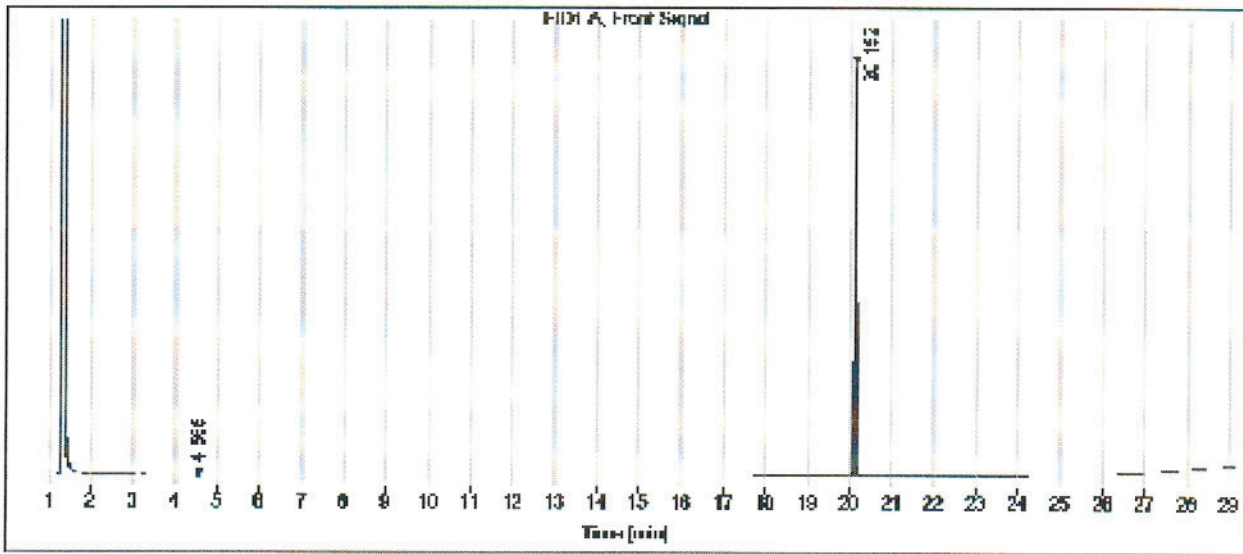

Signal: FID1 A, Front Signal

RT [min]	Type	Width [min]	Area	Height	Area%
4.565	BB	0.0305	1.2408	0.5122	0.11
20.152	BB	0.0391	1171.9556	439.4599	99.89
		Sum	1173.1963		

Chem Service is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015



3050 Spruce Street, Saint Louis, MO 63103, USA  
 Website: [www.sigmaaldrich.com](http://www.sigmaaldrich.com)  
 Email USA: [techserv@sial.com](mailto:techserv@sial.com)  
 Outside USA: [eurtechserv@sial.com](mailto:eurtechserv@sial.com)

## Certificate of Analysis

Product Name:  
 Triacontane-d62 - 98 atom % D

Product Number: 451789  
 Batch Number: MBBC4347  
 Brand: ALDRICH  
 CAS Number: 93952-07-9  
 MDL Number: MFCD00209794  
 Formula: C30D62  
 Formula Weight: 485.20 g/mol  
 Quality Release Date: 27 APR 2018



ID #: 13736

Opened: \_\_\_\_\_


Triacontane-d62-98 atom % D

**Expires: 4/6/2026**

Rec'd: 4/6/2021

Energx Laboratories Inc 1120 So. 27th Street  
 Billings MT 59107

Test	Specification	Result
Purity (HPLC)	≥ 99.0 %	99.0 %
Proton NMR Spectrum	Conforms to Structure	Conforms
D Enrichment	≥ 98.0 %	99.0 %
Initial Melting Point		60.0 °C
Final Melting Point		62.0 °C



Greg Abernathy, Supervisor  
 Quality Control  
 Miamisburg, Ohio US

Sigma-Aldrich warrants, that at the time of the quality release or subsequent retest date this product conformed to the information contained in this publication. The current Specification sheet may be available at Sigma-Aldrich.com. For further inquiries, please contact Technical Service. Purchaser must determine the suitability of the product for its particular use. See reverse side of invoice or packing slip for additional terms and conditions of sale.



# CERTIFIED REFERENCE MATERIAL

110 Benner Circle  
Bellefonte, PA 16823-8812

Tel: (800)356-1688

Fax: (814)353-1309

www.restek.com

## Certificate of Analysis



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

Catalog No. : 31817

Lot No.: A0176667

Description : Residual Range Calibration Standard (RCS)

Residual Range Calib Std (RCS) 50,000µg/mL, Methylene Chloride, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : October 31, 2028

Storage: 25°C nominal

Ship: Ambient

### CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)		
1	Motor Oil SAE30 & SAE40 Blend (Pennzoil) CAS # 64742-65-0.F Purity ----%	50,102.0 µg/mL	+/- 293.3582	µg/mL	Gravimetric
	(Lot A0126386)		+/- 1,492.1008	µg/mL	Unstressed
			+/- 1,591.3244	µg/mL	Stressed

Solvent: Methylene chloride  
CAS # 75-09-2  
Purity 99%

ID #: 14531

Opened: \_\_\_\_\_

Residual Range Calibration Standard

Expires: 10/31/2028

Rec'd: 11/18/2021

Energv Laboratories Inc 1120 So. 27th Street

Billings MT 59107



**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**


250°C

**Det. Temp:**

330°C

**Det. Type:**

FID



This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Sam Moodler*

Sam Moodler - Operations Tech I

Date Mixed: 22-Sep-2021

Balance: 1128360905

*Alexis Shelow*

Alexis Shelow - Operations Tech I

Date Passed: 23-Sep-2021

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value ( includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us) for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us).
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.

# Certificate of Analysis

Diesel Fuel No. 2

*Certified  
Reference  
Material*

## Description

Product ID UST148  
Lot LRAC6316  
Expiration Date April 2023  
Manufacturing Date April 2020  
Storage Conditions Room Temperature  
Solvent/Matrix DICHLOROMETHANE

ID #: 14623

Opened: \_\_\_\_\_

Diesel Fuel No. 2

Expires: 4/30/2023


Rec'd: 12/14/2021

Energy Laboratories Inc 1120 So. 27th Street  
Billings MT 59107

## Certified Values

Analyte	Certified Value <sup>1,4</sup>	Units	Raw Material Purity,%	Raw Material Lot	CAS
NO.2 FUEL OIL	50001 ± 2770	µg/mL	100.0	LA80505	68476-34-6

## Informational Values

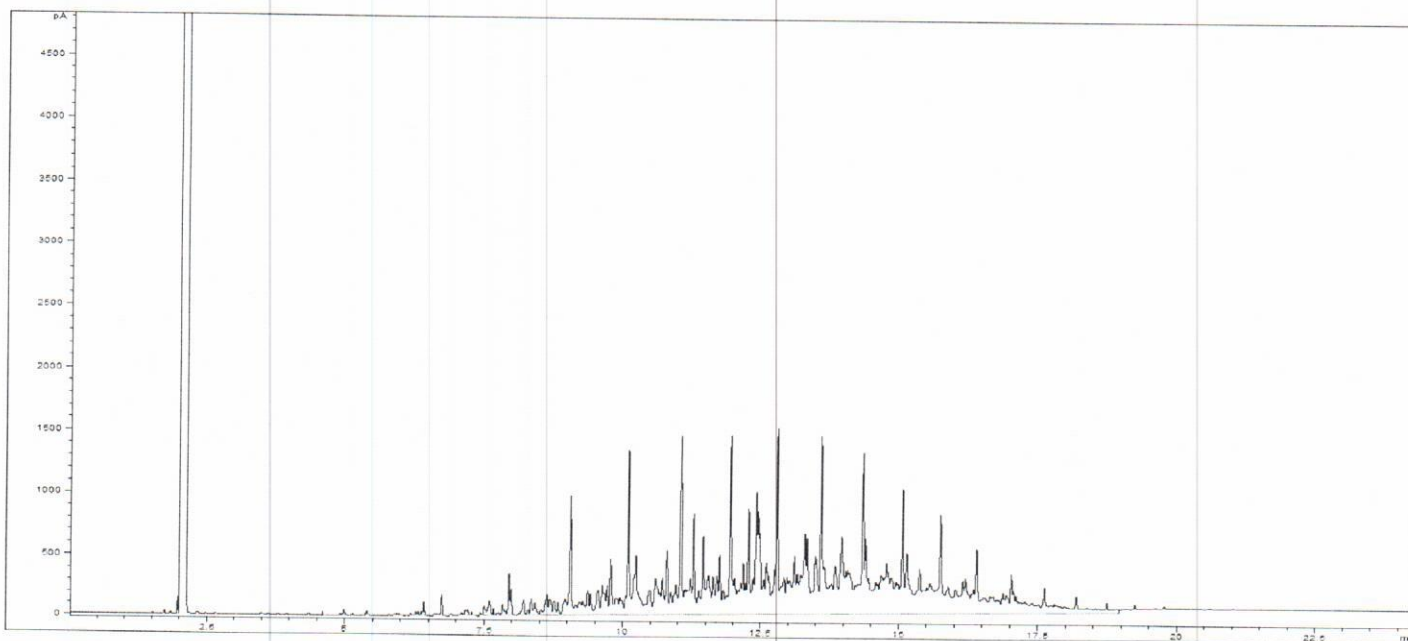

### Additional Information:

Analytical Method Parameters:

Column: SPB-5, 30 m × 0.53 mm I.D., 1.5 µm film thickness (Column #214)

Carrier Gas: H<sub>2</sub>, Flow: 4.0 mL/min

Inlet Temperature: 250 °C, Injection Volume: 1.0 µL

Injection Mode: Split, Split Ratio: 10: 1

Temperature Program: 40 °C (Hold 2 min) @ 15 °C/min to 300 °C (Hold 5 min)

Detector: FID

Detector Temperature: 300 °C



**SIGMA-ALDRICH®**

2931 Soldier Springs Rd. Laramie, Wyoming 82070 USA  
800-325-5832  
TechService@milliporesigma.com www.sigma-aldrich.com



# Description

Lot **LRAC6316**  
Expiration Date April 2023  
Manufacturing Date April 2020  
Storage Conditions Room Temperature  
Solvent/Matrix DICHLOROMETHANE

**1 Metrological traceability:** Traceable to the SI and higher order standards from NIST through an unbroken chain of comparisons. The balance used to weigh raw materials is accurate to +/-0.0001 g and calibrated regularly using mass standards traceable to NIST. All dilutions were performed gravimetrically. Additionally, individual analytes are traceable to NIST SRMs where available and specified above.  
**4 Ucrm - Uncertainty values** in this document are expressed as Expanded Uncertainty (Ucrm) corresponding to the 95% confidence interval. Ucrm is derived from the combined standard uncertainty multiplied by the coverage factor k, which is obtained from a t-distribution and degrees of freedom. The components of combined standard uncertainty include the uncertainties due to characterization, homogeneity, long term stability, and short term stability (transport). The components due to stability are generally considered to be negligible unless otherwise indicated by stability studies. The mathematical representation of the Ucrm calculation is as follows:

$$U_{CRM} = \sqrt{u_{char}^2 + u_{homogeneity}^2 + u_{stability}^2}$$

**k:** Coverage factor derived from a t-distribution table, based on the degrees of freedom of the data set. Assume 2.0 for a **Confidence interval = 95%**

**6 Analytical Value-** For QC verification of the certified value only- not to be used in calculations. Represents the analytical data obtained by comparison to a standard as analyzed by the method described in the CoA or another acceptable method. The result may differ from the certified value and UCRM based on method uncertainty as well as the uncertainty associated with the standard used for comparison.


**Traceability:** The standard was manufactured under an ISO/IEC 17025:2017 certified quality system. The balance used to weigh raw materials is accurate to +/- 0.0001g and calibrated regularly using mass standards traceable to NIST. All dilutions were performed gravimetrically. Additionally, individual analytes are traceable to NIST SRMs where available and specified above.

**Homogeneity:** Homogeneity was assessed in accordance with ISO 17034:2016. Completed units were sampled using a random stratified sampling protocol. The results of chemical analysis were then compared using a one-way analysis of variance approach as described by TNI EL-V3-2009 Appendix A.2. See Instructions for minimum sub-sample size.

Expiration is at end of month given on certificate and label.

MSDS reports for components comprising greater than 1.0% of the solution or 0.1% for components known to be carcinogens are available upon request.

**THIS PRODUCT WAS DESIGNED, PRODUCED AND VERIFIED FOR ACCURACY AND STABILITY IN ACCORDANCE WITH ISO/IEC 17025:2017 (ANAB Cert AT-1467) and ISO 17034:2016 (ANAB Cert AR-1470).**



Andy Ommen - QC Manager

Certification Date April 30, 2020  
Version 0-4302020



Mark Pooler - QA Supervisor







# Analytical RunID GCFID-HP5-B\_220127A Standards Traceability Report

**Standard ID:** DRO200430B  
**Standard Name:** O-Terphenyl  
**Prep Date:** 4/30/2020  
**Exp Date:** 9/30/2024  
**Department:** dropr  
**Vendor:** Chemservice  
**Lot Number:** 9972100  
**Balance ID:**  
**Comments:** ID#: 6271

**Type:** Neat  
**Prep By:** Ann Nebel  
**Status:** New

**Final Volume:** mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
o-Terphenyl	<a href="#">12650</a>	500	mg	9/30/2024
Stock Source	Base Units	Amount Added		



# Analytical RunID GCFID-HP5-B\_220127A Standards Traceability Report

**Standard ID:** DRO210406A

**Standard Name:** Triacontane-d62 Surr For AK103 RRO

**Prep Date:** 4/6/2021

**Exp Date:** 4/6/2026

**Department:** dropr

**Vendor:** Sigma-Aldrich

**Lot Number:** MBBC4347

**Balance ID:**

**Comments:** Alaska surr [for AK103 RRO]

**Type:** Neat

**Prep By:** Ann Nebel

**Status:** New

**Final Volume:** mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Triacontane-d62-98 atom % D	<a href="#">13736</a>	500	mg	4/6/2026
Stock Source	Base Units	Amount Added		



# Analytical RunID GCFID-HP5-B\_220127A Standards Traceability Report

**Standard ID:** DRO211006A

**Standard Name:** Triacontane SURR 2000 ug/mL

**Prep Date:** 10/6/2021

**Exp Date:** 4/6/2026

**Department:** dropr

**Vendor:**

**Lot Number:**

**Balance ID:** BAL-DRO

**Comments:** Triacontane SURR 2000 ug/mL

**Type:** Primary

**Prep By:** Jillian L Bostwick

**Status:** New

**Final Volume:** 50 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Acetone DZ509	<a href="#">13553</a>	50	mL	4/6/2026
Stock Source	Base Units	Amount Added		
DRO210406A	ug/mL	0.1001 g		



# Analytical RunID GCFID-HP5-B\_220127A Standards Traceability Report

**Spike ID:** DRO211101A  
**Spike Name:** OTP-4000 ug/mL DCM  
**Prep Date:** 11/1/2021  
**Exp Date:** 9/30/2024  
**Department:** dropr  
**Vendor:**  
**Lot Number:**  
**Balance ID:** BAL-DRO  
**Comments:** Used to Prep DRO-8015 ICAL and CCV Solutions

**Type:** Secondary  
**Prep By:** Ann Nebel  
**Status:** Open  
**Final Volume:** 25 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Dichloromethane EC328	<a href="#">14408</a>	25	mL	9/30/2024

Stock Source	Base Units	Amount Added
DRO200430B	ug/mL	0.1012 g



# Analytical RunID GCFID-HP5-B\_220127A Standards Traceability Report

**Standard ID:** DRO211118A

**Standard Name:** 50,000 ug/mL Oil Std For AK103 RRO-In DCM

**Prep Date:** 11/18/2021

**Exp Date:** 10/31/2028

**Department:** dropr

**Vendor:** Restek

**Lot Number:** A0176667

**Balance ID:** Sartorius 4 place balance

**Comments:**

**Type:** Primary

**Prep By:** Ann Nebel

**Status:** Open

**Final Volume:** 1 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Residual Range Calibration Standard	<a href="#">14531</a>	1	mL	10/31/2028

Stock Source	Base Units	Amount Added
DRO211118A	ug/mL	



# Analytical RunID GCFID-HP5-B\_220127A Standards Traceability Report

**Standard ID:** DRO211214C

**Standard Name:** Diesel Fuel #2 50,000 ug/mL in DCM

**Prep Date:** 12/14/2021

**Exp Date:** 4/30/2023

**Department:** dropr

**Vendor:** Sigma-Aldrich

**Lot Number:** LRAC6316

**Balance ID:**

**Comments:** Diesel Fuel #2 For CCVs.

**Type:** Primary

**Prep By:** Ann Nebel

**Status:** New

**Final Volume:** mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Diesel Fuel No. 2	<a href="#">14623</a>	1	mL	4/30/2023
Stock Source	Base Units	Amount Added		
DRO211214C	ug/mL			



# Analytical RunID GCFID-HP5-B\_220127A Standards Traceability Report

**Standard ID:** DRO220106B

**Standard Name:** Triacontane SURR 1000 ug/mL

**Prep Date:** 1/6/2022

**Exp Date:** 4/6/2026

**Department:** dropr

**Vendor:**

**Lot Number:**

**Balance ID:** BAL-DRO

**Comments:** 2X dilution of Triacontane SURR 2000 ug/mL

**Type:** Secondary

**Prep By:** Jillian L Bostwick

**Status:** New

**Final Volume:** 10 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Dichloromethane EC832	<a href="#">14647</a>	5	mL	4/6/2026

Stock Source	Base Units	Amount Added
DRO211006A	ug/mL	5 mL



# Analytical RunID GCFID-HP5-B\_220127A Standards Traceability Report

**Standard ID:** DRO220110A

**Standard Name:** Carbon Scan STD-Marker

**Prep Date:** 1/11/2022

**Exp Date:** 7/13/2026

**Department:** dropr

**Vendor:** ASI2

**Lot Number:** 55064

**Balance ID:**

**Comments:** FOR Qualitative analyst only.31 compounds-C5 to C30,32,34,36,38,40.

**Type:** Neat

**Prep By:** Ann Nebel

**Status:** Open

**Final Volume:** 1.2 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
n-Hydrocarbons- C5 to C30, C32, C34, C36, C38, C40	<a href="#">14737</a>	1.2	mL	7/13/2026

Stock Source	Base Units	Amount Added
DRO220110A	ug/mL	





# Analytical RunID GCFID-HP5-B\_220127A Standards Traceability Report

**Standard ID:** DRO220111A

**Standard Name:** Carbon Scan STD-Marker

**Prep Date:** 1/11/2022

**Exp Date:** 7/13/2026

**Department:** dropr

**Vendor:** ASI2

**Lot Number:** 071306

**Balance ID:**

**Comments:** FOR Qualitative analyst only.31 compounds-C5 to C30,32,34,36,38,40.

**Type:** Primary

**Prep By:** Ann Nebel

**Status:** Open

**Final Volume:** 2.4 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Carbon Disulfide 55064	<a href="#">7477</a>	1.2	mL	7/13/2026

Stock Source	Base Units	Amount Added
DRO220110A	ug/mL	1.2 mL



# Analytical RunID GCFID-HP5-B\_220127A Standards Traceability Report

**Standard ID:** DRO220118A

**Standard Name:** 5,000 ug/mL RRO CCV 200 ug/mL Triacontane

**Prep Date:** 1/18/2022

**Exp Date:** 4/6/2026

**Department:** dropr

**Vendor:**

**Lot Number:**

**Balance ID:**

**Comments:** CCV for AK102 and 8015C RRO.

**Type:** Secondary

**Prep By:** Ann Nebel

**Status:** New

**Final Volume:** 4 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Dichloromethane EC849	<a href="#">14747</a>	2.8	mL	4/6/2026

Stock Source	Base Units	Amount Added
DRO220106B	ug/mL	800 µL
DRO211118A	ug/mL	400 µL



# Analytical RunID GCFID-HP5-B\_220127A Standards Traceability Report

**Standard ID:** DRO220124A

**Standard Name:** 8015 CCV-15,000ug/mL + 200 OTP

**Prep Date:** 1/24/2022

**Exp Date:** 4/30/2023

**Department:** dropr

**Vendor:**

**Lot Number:**

**Balance ID:**

**Comments:** 8015DRO CCV MIX-15,000ug/mL +200 OTP #2 Diesel

**Type:** Secondary

**Prep By:** Jillian L Bostwick

**Status:** New

**Final Volume:** 4 mL

Chemical/Solvent Used	Bottle No	Amt	Units	Expires
Dichloromethane EC849	<a href="#">14747</a>	2.6	mL	4/30/2023

Stock Source	Base Units	Amount Added
DRO211214C	ug/mL	1.2 mL
DRO211101A	ug/mL	0.2 mL

Anna

660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599  
1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729  
[info@chemservice.com](mailto:info@chemservice.com) • [www.chemservice.com](http://www.chemservice.com)

## CERTIFICATE OF ANALYSIS

### o-Terphenyl

CATALOG NUMBER N-12693-500MG  
LOT NUMBER 9972100  
DATE CERTIFIED 09/23/19  
EXPIRATION DATE 09/30/24  
CAS NUMBER 84-15-1  
MOLECULAR FORMULA C18H14  
MOLECULAR WEIGHT 230.32  
STORAGE Store in a cool dry place.  
HANDLING See Safety Data Sheet  
INTENDED USE For laboratory use only.

Analytical Test	Value
FT-IR SPECTROSCOPY	CONFORMS TO STRUCTURE
GC/MS SPECTRA ID	MATCHES NIST DATABASE
MELTING POINT (°C)	57.1
% PURITY (GC/FID)	99.5

Chem Service, Inc. guarantees the purity to be +/- 0.5% deviation prior to the expiration date shown on the label and exclusive of any customer contamination.

Certified By:

*Mary Beth O'Donnell*

Mary Beth O'Donnell  
CSM/TC

ID #: 12650

Opened: \_\_\_\_\_

o-Terphenyl

Expires: 9/30/2024

Rec'd: 4/30/2020

Energyl Laboratories Inc 1120 So. 27th Street

Billings MT 59107

COA Form  
Revision 3 (3/2015)


Chem Service is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015



## CERTIFICATE OF ANALYSIS

### Analysis Method:

Catalog Number: N-12693-500MG  
Description: o-Terphenyl  
Lot Number: 9972100  
Expiration Date: 09/30/24



Chem Service is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015



## CERTIFICATE OF ANALYSIS

### Analysis Method:

Catalog Number: N-12693-500MG  
Description: o-Terphenyl  
Lot Number: 9972100  
Expiration Date: 09/30/24

Chem Service Inc      Area Percent Report

Data File: D:\msdchem\2019 DATA\0919\0923-01.D  
Acq On : 23 Sep 2019 10:40  
Operator :  
Sample : n-12693  
Misc :  
ALS Vial : 95

Integration Parameters: autoint1.e  
Integrator: ChemStation

DataAcq Meth: SCREEN.M  
Method : D:\msdchem\2019 DATA\0919\0903-09.D\ERIN.M

Signal : TIC: 0923-01.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	11.844	1597	1606	1613	BB	32038221	432253484	100.00%	100.000%

Sum of corrected areas: 432253484

ERIN.M Mon Sep 23 10:55:51 2019




660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599  
1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729  
[info@chemservice.com](mailto:info@chemservice.com) • [www.chemservice.com](http://www.chemservice.com)

## CERTIFICATE OF ANALYSIS


### Analysis Method:

Catalog Number: N-12693-500MG  
Description: o-Terphenyl  
Lot Number: 9972100  
Expiration Date: 09/30/24

Abundance

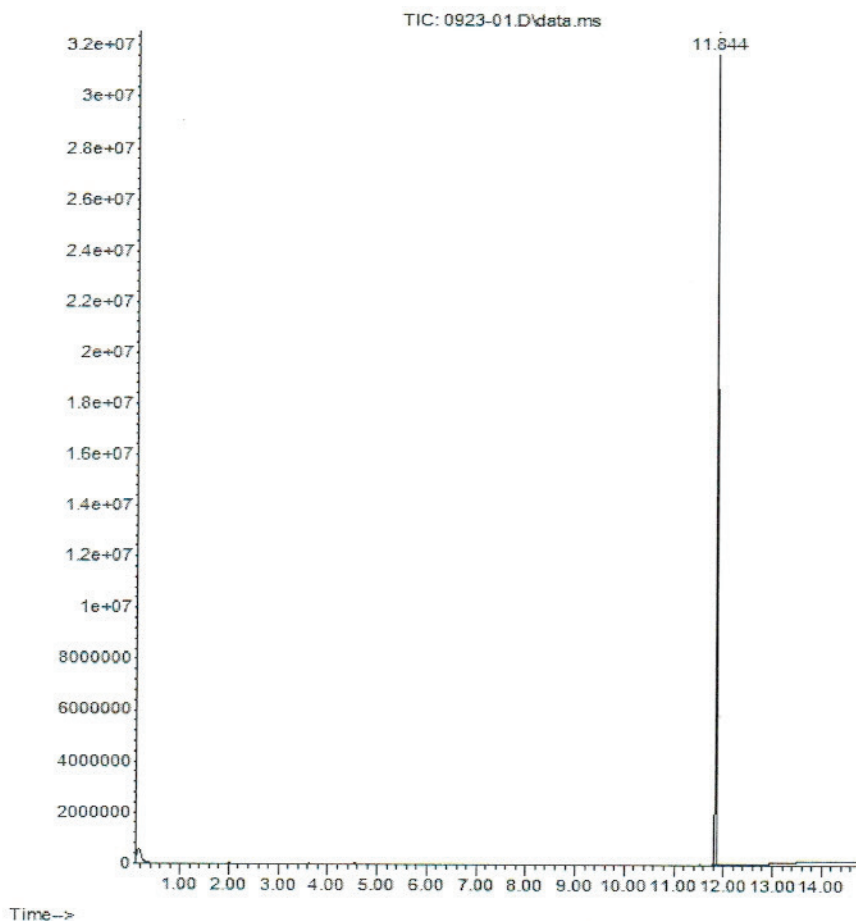

Chem Service is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015




660 Tower Lane • P. O. Box 599 • West Chester, PA 19381-0599  
1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729  
[info@chemservice.com](mailto:info@chemservice.com) • [www.chemservice.com](http://www.chemservice.com)

## CERTIFICATE OF ANALYSIS

### Analysis Method:

Catalog Number: N-12693-500MG  
Description: o-Terphenyl  
Lot Number: 9972100  
Expiration Date: 09/30/24

Abundance



Chem Service is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015.





660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599  
1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729  
[info@chemservice.com](mailto:info@chemservice.com) • [www.chemservice.com](http://www.chemservice.com)

## CERTIFICATE OF ANALYSIS

### Analysis Method:

Catalog Number:	N-12693-500MG
Description:	o-Terphenyl
Lot Number:	9972100
Expiration Date:	09/30/24

Chem Service is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015




660 Tower Lane • P.O. Box 599 • West Chester, PA 19381-0599  
 1-800-452-9994 • 1-610-692-3026 • Fax 1-610-692-8729  
[info@chemservice.com](mailto:info@chemservice.com) • [www.chemservice.com](http://www.chemservice.com)

Gas

Data file: C:\CHEM3\  
 Sample name: N-12893  
 Instrument: GC 2  
 Injection date: 8/23/2019 9:58:34 AM  
 Acq. method: SCREEN.M  
 Column name: HP-5

## CERTIFICATE OF ANALYSIS

Location: Vial 141  
 Injection volume: 1.0uL

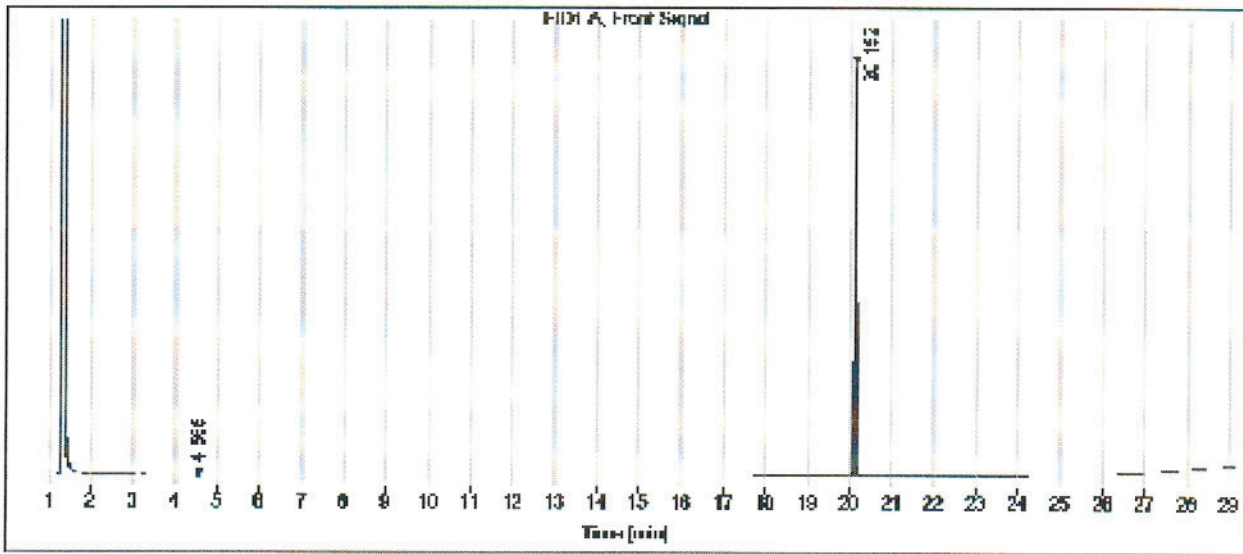

Signal: FID1 A, Front Signal

RT [min]	Type	Width [min]	Area	Height	Area%
4.565	BB	0.0305	1.2408	0.5122	0.11
20.152	BB	0.0391	1171.9556	439.4599	99.89
		Sum	1173.1963		

Chem Service is accredited to ISO 17034:2016, ISO/IEC 17025:2017 and certified to ISO 9001:2015



3050 Spruce Street, Saint Louis, MO 63103, USA  
 Website: www.sigmaaldrich.com  
 Email USA: techserv@sial.com  
 Outside USA: eurtechserv@sial.com

## Certificate of Analysis

Product Name:  
 Triacontane-d62 - 98 atom % D

Product Number: 451789  
 Batch Number: MBBC4347  
 Brand: ALDRICH  
 CAS Number: 93952-07-9  
 MDL Number: MFCD00209794  
 Formula: C30D62  
 Formula Weight: 485.20 g/mol  
 Quality Release Date: 27 APR 2018



ID #: 13736

Opened: \_\_\_\_\_


Triacontane-d62-98 atom % D

Expires: 4/6/2026

Rec'd: 4/6/2021

Energx Laboratories Inc 1120 So. 27th Street  
 Billings MT 59107

Test	Specification	Result
Purity (HPLC)	≥ 99.0 %	99.0 %
Proton NMR Spectrum	Conforms to Structure	Conforms
D Enrichment	≥ 98.0 %	99.0 %
Initial Melting Point		60.0 °C
Final Melting Point		62.0 °C



Greg Abernathy, Supervisor  
 Quality Control  
 Miamisburg, Ohio US

Sigma-Aldrich warrants, that at the time of the quality release or subsequent retest date this product conformed to the information contained in this publication. The current Specification sheet may be available at Sigma-Aldrich.com. For further inquiries, please contact Technical Service. Purchaser must determine the suitability of the product for its particular use. See reverse side of invoice or packing slip for additional terms and conditions of sale.



# CERTIFIED REFERENCE MATERIAL

110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

## Certificate of Analysis



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 31817 **Lot No.:** A0176667

**Description :** Residual Range Calibration Standard (RCS)

Residual Range Calib Std (RCS) 50,000µg/mL, Methylene Chloride, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** October 31, 2028 **Storage:** 25°C nominal

**Ship:** Ambient

### CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)	
1	Motor Oil SAE30 & SAE40 Blend (Pennzoil) CAS # 64742-65-0.F Purity ----%	50,102.0 µg/mL	+/- 293.3582 µg/mL +/- 1,492.1008 µg/mL +/- 1,591.3244 µg/mL	Gravimetric Unstressed Stressed

**Solvent:** Methylene chloride  
CAS # 75-09-2  
Purity 99%

ID #: 14531

Opened: \_\_\_\_\_

Residual Range Calibration Standard

**Expires: 10/31/2028**

Rec'd: 11/18/2021

Energ Laboratories Inc 1120 So. 27th Street  
Billings MT 59107



**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**


250°C

**Det. Temp:**

330°C

**Det. Type:**

FID



This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Sam Moodler*

Sam Moodler - Operations Tech I

Date Mixed: 22-Sep-2021

Balance: 1128360905

*Alexis Shelow*

Alexis Shelow - Operations Tech I

Date Passed: 23-Sep-2021

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

## General Certified Reference Material Notes

### Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

### Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ $\mu$ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

### Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified combined stressed uncertainty value ( includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{combined\ stressed} = k \sqrt{U_{gravimetric}^2 + U_{homogeneity}^2 + U_{storage\ stability}^2 + U_{shipping\ stability}^2}$$

$k$  is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- It is important to note that the shipping stability uncertainty was obtained under temperature extremes for specific time intervals; therefore, the certified combined stressed uncertainty value should only be applied to the product if it was stored at non-standard temperature conditions up to and including 7 days. Contact Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us) for use recommendations if your shipment was in-transit for more than 7 days at non-standard temperature conditions.
- Apply the certified combined unstressed uncertainty value if the product was received under standard shipping conditions. Apply the certified combined stressed uncertainty value if the product was received under non-standard conditions as specified below.

Label Conditions	Standard Conditions	Non-Standard Conditions
25°C Nominal (Room Temperature)	< 60°C	≥ 60°C up to 7 days
10°C or colder (Refrigerate)	< 40°C	≥ 40°C up to 7 days
0°C or colder (Freezer) -20°C or colder (Deep Freezer)	< 25°C	≥ 25°C up to 7 days

- Separate (not combined) uncertainty values for gravimetric uncertainty are also displayed on the certificate, if needed, separate homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty values are available by contacting Restek Technical Service at [www.restek.com/Contact-Us](http://www.restek.com/Contact-Us).
- The packaged amount is the minimum sample size for which uncertainty is valid. The ampules are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

### Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

### Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampules. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.

# Certificate of Analysis

Diesel Fuel No. 2

*Certified  
Reference  
Material*

## Description

Product ID UST148  
Lot LRAC6316  
Expiration Date April 2023  
Manufacturing Date April 2020  
Storage Conditions Room Temperature  
Solvent/Matrix DICHLOROMETHANE

ID #: 14623

Opened: \_\_\_\_\_

Diesel Fuel No. 2

Expires: 4/30/2023


Rec'd: 12/14/2021

Energy Laboratories Inc 1120 So. 27th Street  
Billings MT 59107

## Certified Values

Analyte	Certified Value <sup>1,4</sup>	Units	Raw Material Purity,%	Raw Material Lot	CAS
NO.2 FUEL OIL	50001 ± 2770	µg/mL	100.0	LA80505	68476-34-6

## Informational Values



## Additional Information:

Analytical Method Parameters:

Column: SPB-5, 30 m × 0.53 mm I.D., 1.5 µm film thickness (Column #214)

Carrier Gas: H<sub>2</sub>, Flow: 4.0 mL/min

Inlet Temperature: 250 °C, Injection Volume: 1.0 µL

Injection Mode: Split, Split Ratio: 10: 1

Temperature Program: 40 °C (Hold 2 min) @ 15 °C/min to 300 °C (Hold 5 min)

Detector: FID

Detector Temperature: 300 °C



**SIGMA-ALDRICH®**

2931 Soldier Springs Rd. Laramie, Wyoming 82070 USA  
800-325-5832  
TechService@milliporesigma.com www.sigma-aldrich.com



# Description

Lot **LRAC6316**  
Expiration Date April 2023  
Manufacturing Date April 2020  
Storage Conditions Room Temperature  
Solvent/Matrix DICHLOROMETHANE

**1 Metrological traceability:** Traceable to the SI and higher order standards from NIST through an unbroken chain of comparisons. The balance used to weigh raw materials is accurate to +/-0.0001 g and calibrated regularly using mass standards traceable to NIST. All dilutions were performed gravimetrically. Additionally, individual analytes are traceable to NIST SRMs where available and specified above.  
**4 Ucrm - Uncertainty values** in this document are expressed as Expanded Uncertainty (Ucrm) corresponding to the 95% confidence interval. Ucrm is derived from the combined standard uncertainty multiplied by the coverage factor k, which is obtained from a t-distribution and degrees of freedom. The components of combined standard uncertainty include the uncertainties due to characterization, homogeneity, long term stability, and short term stability (transport). The components due to stability are generally considered to be negligible unless otherwise indicated by stability studies. The mathematical representation of the Ucrm calculation is as follows:

$$U_{CRM} = \sqrt{u_{char}^2 + u_{homogeneity}^2 + u_{stability}^2}$$

**k:** Coverage factor derived from a t-distribution table, based on the degrees of freedom of the data set. Assume 2.0 for a **Confidence interval = 95%**

**6 Analytical Value-** For QC verification of the certified value only- not to be used in calculations. Represents the analytical data obtained by comparison to a standard as analyzed by the method described in the CoA or another acceptable method. The result may differ from the certified value and UCRM based on method uncertainty as well as the uncertainty associated with the standard used for comparison.


**Traceability:** The standard was manufactured under an ISO/IEC 17025:2017 certified quality system. The balance used to weigh raw materials is accurate to +/- 0.0001g and calibrated regularly using mass standards traceable to NIST. All dilutions were performed gravimetrically. Additionally, individual analytes are traceable to NIST SRMs where available and specified above.

**Homogeneity:** Homogeneity was assessed in accordance with ISO 17034:2016. Completed units were sampled using a random stratified sampling protocol. The results of chemical analysis were then compared using a one-way analysis of variance approach as described by TNI EL-V3-2009 Appendix A.2. See Instructions for minimum sub-sample size.

Expiration is at end of month given on certificate and label.

MSDS reports for components comprising greater than 1.0% of the solution or 0.1% for components known to be carcinogens are available upon request.

**THIS PRODUCT WAS DESIGNED, PRODUCED AND VERIFIED FOR ACCURACY AND STABILITY IN ACCORDANCE WITH ISO/IEC 17025:2017 (ANAB Cert AT-1467) and ISO 17034:2016 (ANAB Cert AR-1470).**



Andy Ommen - QC Manager

Certification Date April 30, 2020  
Version 0-4302020



Mark Pooler - QA Supervisor

